

---

**ADVANTEST**<sup>®</sup>  
ADVANTEST CORPORATION

---

**Q8384**

***Optical Spectrum Analyzer***

***Operation Manual***

MANUAL NUMBER FOE-8335041D00

---

## Safety Summary

To ensure thorough understanding of all functions and to ensure efficient use of this instrument, please read the manual carefully before using. Note that Advantest bears absolutely no responsibility for the result of operations caused due to incorrect or inappropriate use of this instrument.

If the equipment is used in a manner not specified by Advantest, the protection provided by the equipment may be impaired.

### • Warning Labels

Warning labels are applied to Advantest products in locations where specific dangers exist. Pay careful attention to these labels during handling. Do not remove or tear these labels. If you have any questions regarding warning labels, please ask your nearest Advantest dealer. Our address and phone number are listed at the end of this manual.

Symbols of those warning labels are shown below together with their meaning.

**DANGER:** Indicates an imminently hazardous situation which will result in death or serious personal injury.

**WARNING:** Indicates a potentially hazardous situation which will result in death or serious personal injury.

**CAUTION:** Indicates a potentially hazardous situation which will result in personal injury or a damage to property including the product.

### • Basic Precautions

Please observe the following precautions to prevent fire, burn, electric shock, and personal injury.

- Use a power cable rated for the voltage in question. Be sure however to use a power cable conforming to safety standards of your nation when using a product overseas.
- When inserting the plug into the electrical outlet, first turn the power switch OFF and then insert the plug as far as it will go.
- When removing the plug from the electrical outlet, first turn the power switch OFF and then pull it out by gripping the plug. Do not pull on the power cable itself. Make sure your hands are dry at this time.
- Before turning on the power, be sure to check that the supply voltage matches the voltage requirements of the instrument.
- Be sure to plug the power cable into an electrical outlet which has a safety ground terminal. Grounding will be defeated if you use an extension cord which does not include a safety ground terminal.
- Be sure to use fuses rated for the voltage in question.
- Do not use this instrument with the case open.

---

## Safety Summary

- Do not place objects on top of this product. Also, do not place flower pots or other containers containing liquid such as chemicals near this product.
  - When the product has ventilation outlets, do not stick or drop metal or easily flammable objects into the ventilation outlets.
  - When using the product on a cart, fix it with belts to avoid its drop.
  - When connecting the product to peripheral equipment, turn the power off.
- **Caution Symbols Used Within this Manual**

Symbols indicating items requiring caution which are used in this manual are shown below together with their meaning.

**DANGER:** Indicates an item where there is a danger of serious personal injury (death or serious injury).


**WARNING:** Indicates an item relating to personal safety or health.

**CAUTION:** Indicates an item relating to possible damage to the product or instrument or relating to a restriction on operation.


- **Safety Marks on the Product**

The following safety marks can be found on Advantest products.

 : ATTENTION - Refer to manual.

 : Protective ground (earth) terminal.

 : DANGER - High voltage.

 : CAUTION - Risk of electric shock.

• **Replacing Parts with Limited Life**

The following parts used in the instrument are main parts with limited life. Replace the parts listed below after their expected lifespan has expired. Note that the estimated lifespan for the parts listed below may be shortened by factors such as the environment where the instrument is stored or used, and how often the instrument is used.

There is a possibility that each product uses different parts with limited life. For more information, refer to Chapter 1.

Main Parts with Limited Life

Part name	Life
Unit power supply	5 years
Fan motor	5 years
Electrolytic capacitor	5 years
LCD panel	6 years
LCD backlight	2.5 years
Floppy disk drive	5 years

• **Precautions when Disposing of this Instrument**

When disposing of harmful substances, be sure dispose of them properly with abiding by the state-provided law.

- Harmful substances:
- (1) PCB (polycarbon biphenyl)
  - (2) Mercury
  - (3) Ni-Cd (nickel cadmium)
  - (4) Other
    - Items possessing cyan, organic phosphorous and hexadic chromium and items which may leak cadmium or arsenic (excluding lead in solder).


Example: fluorescent tubes, batteries

---

# Environmental Conditions


This instrument should only be used in an area which satisfies the following conditions:

- An area free from corrosive gas
- An area away from direct sunlight
- A dust-free area
- An area free from vibrations

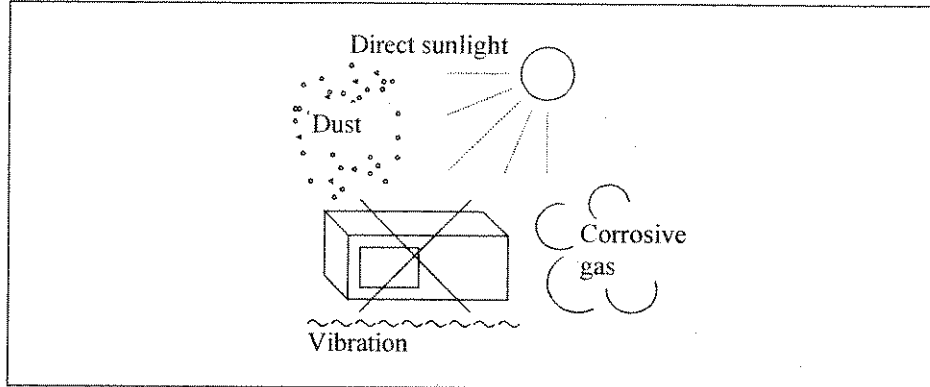

**Figure-1 Environmental Conditions**

- Instrument Placement

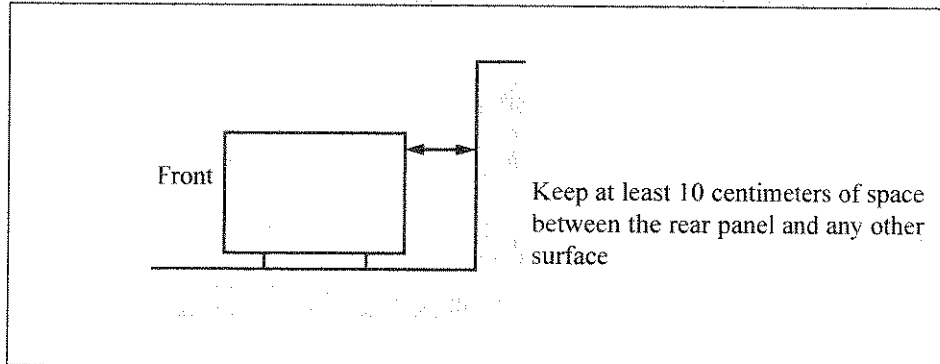

**Figure-2 Instrument Placement**

This instrument can be used safely under the following conditions:

- Altitude of up to 2000 m
- Installation Categories II
- Pollution Degree 2

# Certificate of Conformity



This is to certify, that

**Optical Spectrum Analyzer**

---

**Q8384**

---

instrument, type, designation

complies with the provisions of the EMC Directive 89/336/EEC in accordance with EN50081-1 and EN50082-1 and Low Voltage Directive 73/23/EEC in accordance with EN61010.

**ADVANTEST Corp.**

Tokyo, Japan

**ROHDE&SCHWARZ**

Engineering and Sales GmbH  
Munich, Germany

## PREFACE

This manual provides the information necessary to check functionality, operate and program the Q8384 Optical Spectrum Analyzer Operation. Be sure to read this manual carefully in order to use the Optical Spectrum Analyzer safely.

- Organization of this manual  
This manual consists of the following chapters:

<p>1. Introduction</p> <ul style="list-style-type: none"> <li>• Product Description</li> <li>• Standard Accessories and Power Cable Options</li> <li>• Operating Environment</li> <li>• Operation Check</li> <li>• Setting the Print Paper</li> <li>• Cleaning, Storing and Transporting</li> </ul>	<p>Includes a description of the Optical Spectrum Analyzer and its' parts along with information on its' operating environment and how to perform a system checkout.</p>
<p>2. Operation</p> <ul style="list-style-type: none"> <li>• Controls and Connectors on the Front and Rear Panels</li> <li>• Screen Annotation</li> <li>• Basic Operation</li> <li>• Measurement Examples</li> <li>• Expanded Functions</li> </ul>	<p>Describes the names and the functions of each part on the panels. You can learn the basic operation of the Optical Spectrum Analyzer through the examples shown in this chapter.</p>
<p>3. Reference</p> <ul style="list-style-type: none"> <li>• Menu Index</li> <li>• Menu Map</li> <li>• Functional Description</li> </ul>	<p>Shows a list of operation keys, and describes the function of each key.</p>
<p>4. Remote Control</p> <ul style="list-style-type: none"> <li>• GPIB</li> </ul>	<p>Gives an outline of the GPIB interface, and how to connect and set them up. Also included are a list of commands necessary for programming and using the program examples.</p>
<p>5. Technical Notes</p> <ul style="list-style-type: none"> <li>• Technical Notes</li> <li>• Operation Principle</li> <li>• Block Diagram</li> </ul>	<p>Describes the principle of operation necessary for taking measurements more accurately.</p>
<p>6. Specifications</p>	<p>Shows the specifications of the Optical Spectrum Analyzer.</p>
<p>Appendix</p> <ul style="list-style-type: none"> <li>• Glossary</li> </ul>	<p>Terminology related to the Optical Spectrum Analyzer is explained in this section.</p>

Preface

- Key notations in this manual  
Typeface conventions used in this manual.

Panel keys: In bold type

Example: **MAG, SYSTEM**

Soft keys: In bold and italic type

Example: ***CENTER, PRESET***



## TABLE OF CONTENTS

1	INTRODUCTION .....	1-1
1.1	Product Overview .....	1-1
1.2	Accessories, Option and Limited-life Part .....	1-2
1.2.1	Standard Accessories .....	1-2
1.2.2	Option and Accessories .....	1-2
1.2.3	Limited-life Part .....	1-2
1.3	Operating Environment .....	1-4
1.3.1	Environmental Conditions .....	1-4
1.3.2	Power Requirements .....	1-5
1.3.3	Power Fuse .....	1-6
1.3.4	Power Cable .....	1-7
1.4	System Checkout .....	1-8
1.5	Setting the Print Paper .....	1-9
1.6	Cleaning, Storing and Transporting the Q8384 Optical Spectrum Analyzer .....	1-10
1.6.1	Cleaning .....	1-10
1.6.2	Storing .....	1-10
1.6.3	Replacing and Cleaning the Optical-Connector Adapter of Q8384 .....	1-11
1.6.4	Transporting .....	1-12
1.7	Warm-up time .....	1-12
1.8	About Calibration .....	1-12
2	OPERATION .....	2-1
2.1	Panel Description .....	2-1
2.1.1	Front Panel .....	2-1
2.1.1.1	LCD Display Section .....	2-2
2.1.1.2	FUNCTION Section .....	2-3
2.1.1.3	CURSOR Section .....	2-4
2.1.1.4	MEASURE Section .....	2-4
2.1.1.5	DATA Section .....	2-5
2.1.1.6	DISPLAY Section .....	2-6
2.1.1.7	DATA OUT Section .....	2-7
2.1.1.8	GP-IB Section .....	2-7
2.1.1.9	Connector Section .....	2-8
2.1.1.10	POWER Switch/Floppy Disk Drive Section .....	2-8
2.1.2	Screen Annotation .....	2-9
2.1.3	Rear Panel .....	2-11
2.2	Basic Operation .....	2-12
2.2.1	Operating Menus and Entering Data .....	2-12
2.2.2	Light Spectrum Measurement .....	2-14
2.2.3	Peak Power Monitor Measurement .....	2-21
2.2.4	Alignment .....	2-24

## Table of Contents

2.2.5	Calibration .....	2-26
2.2.6	Measuring the Transmission-wavelength (or Loss-wavelength) Characteristics .....	2-29
2.2.7	Light Amplifier Characteristic Analysis .....	2-33
2.2.8	WDM Light Signal Characteristic Analysis .....	2-37
2.2.9	WDM Optical Signal Measurements Using the Monitoring Function .....	2-41
2.2.10	Limit Line Function for Device Evaluation .....	2-48
2.2.11	Setting Measurement Conditions .....	2-51
2.3	Using Expanded Functions and Inputting/Outputting Data .....	2-57
2.3.1	Entering Label Data .....	2-57
2.3.2	Selecting Color Patterns on the Screen .....	2-58
2.3.3	Setting Date/Time .....	2-58
2.3.4	Saving or Reading Data .....	2-59
2.3.4.1	Floppy Disk .....	2-59
2.3.4.2	Backup Memory .....	2-60
2.3.4.3	Saving Data .....	2-60
2.3.4.4	Reading Data .....	2-61
2.3.5	Outputting Data (Hard Copy) .....	2-62
2.3.5.1	Internal printer .....	2-62
2.3.5.2	External printer .....	2-62
2.3.5.3	Floppy disk .....	2-63
3	REFERENCE .....	3-1
3.1	Menu Index .....	3-1
3.2	Menu Map .....	3-5
3.3	Functional Description .....	3-15
3.3.1	CENTER Key .....	3-15
3.3.2	SPAN Key .....	3-16
3.3.3	REF LEVEL Key .....	3-17
3.3.4	LEVEL SCALE Key .....	3-18
3.3.5	RESOLUTION Key .....	3-19
3.3.6	SWEEP MODE Key .....	3-20
3.3.7	AVG Key .....	3-22
3.3.8	AUTO Key .....	3-23
3.3.9	SINGLE Key .....	3-23
3.3.10	REPEAT Key .....	3-23
3.3.11	STOP Key .....	3-23
3.3.12	NORMALIZE LOSS/TRANS Key .....	3-24
3.3.13	APPLICATION Key .....	3-25
3.3.14	ADVANCE Key .....	3-33
3.3.15	ON/OFF Key .....	3-34
3.3.16	$\lambda_1$ Key .....	3-34
3.3.17	$\lambda_2$ Key .....	3-34
3.3.18	L1 Key .....	3-34

3.3.19	L2 Key .....	3-34
3.3.20	CONTROL Key .....	3-35
3.3.21	SAVE Key .....	3-37
3.3.22	RECALL Key .....	3-38
3.3.23	DEVICE Key .....	3-39
3.3.24	COPY Key .....	3-42
3.3.25	FEED Key .....	3-42
3.3.26	LOCAL Key .....	3-42
3.3.27	INSTR PRESET Key .....	3-42
3.3.28	CAL Key .....	3-43
3.3.29	LABEL Key .....	3-44
3.4	List of Settings .....	3-45
3.4.1	Defaults Configuration Values .....	3-45
4	REMOTE CONTROL .....	4-1
4.1	GPIB Command Index .....	4-1
4.2	Overview of GPIB .....	4-3
4.3	Interface Functions .....	4-4
4.4	Program Code .....	4-5
4.5	Talker Formats (Data Output Formats) .....	4-6
4.6	Device Triggering Function .....	4-26
4.7	Device Clear Function .....	4-26
4.8	State Changes According to the Commands .....	4-27
4.9	Status Byte .....	4-28
4.10	GPIB Command Codes .....	4-29
4.11	Example Programs .....	4-41
4.11.1	Sample Programs for Setting or Reading Measurement Conditions .....	4-41
5	TECHNICAL NOTES .....	5-1
5.1	Measurement Modes .....	5-1
5.2	Averaging Functions .....	5-2
5.3	Calculating the Spectral Width and the Notch Width .....	5-3
5.3.1	Calculating the Spectral Width .....	5-3
5.3.1.1	PEAK THRESHOLD .....	5-3
5.3.1.2	ENVELOPE .....	5-4
5.3.1.3	RMS .....	5-4
5.3.1.4	Peak RMS .....	5-5
5.3.1.5	Xnm Level .....	5-5
5.3.2	Notch Width .....	5-6
5.3.2.1	XdB WIDTH .....	5-6
5.3.2.2	Xnm Level .....	5-7
5.4	GAIN&NF and SNR .....	5-8
5.4.1	GAIN .....	5-9

Table of Contents

5.4.2	NF .....	5-10
5.4.3	SPE DIV .....	5-11
5.5	Auto-Panning and Auto-Zooming Functions .....	5-12
5.6	Cursor Modes and Explanation for Displayed Data .....	5-13
5.7	Setting Limit Line .....	5-14
5.7.1	Data Files .....	5-14
5.7.2	Limit Line Data .....	5-14
5.8	Operation Principle .....	5-18
5.9	Notes on Using the Optical Spectrum Analyzer .....	5-21
5.9.1	Optical Fibers Suitable for the Optical Spectrum Analyzer .....	5-21
5.9.2	Stray Light .....	5-21
5.9.3	Secondary Diffracted Light .....	5-21
6	SPECIFICATIONS .....	6-1
APPENDIX .....		A-1
A.1	Glossary .....	A-1
A.2	Error Messages .....	A-11
A.3	Other Messages .....	A-12
A.4	Example of a Spectrum Data File on a Floppy Disk .....	A-12
DIMENSIONAL OUTLINE DRAWING .....		EXT-1
ALPHABETICAL INDEX .....		I-1

## LIST OF ILLUSTRATIONS

No.	Title	Page
1-1	Operating Environment .....	1-4
1-2	Replacing the Power Fuse .....	1-6
1-3	Power Cable .....	1-7
1-4	Setting the Print Paper .....	1-9
1-5	Replacing and Cleaning the Optical-connector Adapter .....	1-11
2-1	Front Panel .....	2-1
2-2	LCD Display Section .....	2-2
2-3	FUNCTION Section .....	2-3
2-4	CURSOR Section .....	2-4
2-5	MEASURE Section .....	2-4
2-6	DATA Section .....	2-5
2-7	DISPLAY Section .....	2-6
2-8	DATA OUT Section .....	2-7
2-9	GP-IB Section .....	2-7
2-10	Connector Section .....	2-8
2-11	POWER Switch and Floppy Disk Drive Section .....	2-8
2-12	Screen Annotation .....	2-9
2-13	Rear Panel .....	2-11
2-14	CENTER Menu .....	2-12
2-15	Self-test Screen .....	2-14
2-16	INSTR PRESET Menu .....	2-15
2-17	Light Spectrum Measurement .....	2-15
2-18	Input Window .....	2-16
2-19	Setting the Center Wavelength .....	2-16
2-20	Displaying the Spectrum .....	2-17
2-21	Peak Search .....	2-18
2-22	Changing the Center Wavelength .....	2-18
2-23	Displaying the Cursor .....	2-19
2-24	Setting the Analysis Span .....	2-19
2-25	Setting the Analysis Span-1 .....	2-20
2-26	Setting the Analysis Span-2 .....	2-20
2-27	Peak Power Monitor Measurement .....	2-21
2-28	Displaying the Spectrum .....	2-22
2-29	Displaying Input Light Changes in Time .....	2-23
2-30	Connecting the Calibration Signal .....	2-24
2-31	Alignment Execution Message .....	2-25
2-32	Connecting the Calibration Signal .....	2-26
2-33	Calibration Execution Message .....	2-27
2-34	Connecting the Calibration Signal .....	2-28
2-35	Calibration Execution Message .....	2-28
2-36	Connecting the White Light Source .....	2-29
2-37	Saving the Reference Spectrum .....	2-30
2-38	Connecting the White Light Source .....	2-30
2-39	Transmission-wavelength Characteristics (Zooming function with LOSS/TRANS) .....	2-31

## List of Illustrations

No.	Title	Page
2-40	Loss-wavelength Characteristics (Zooming function with LOSS/TRANS) .....	2-31
2-41	Measuring the Input Signal .....	2-34
2-42	Saving the REF Data .....	2-34
2-43	Measuring the Output Signal .....	2-35
2-44	Optical AMP PARAMETER Dialog Box .....	2-35
2-45	Input Signal Connections .....	2-37
2-46	Measuring the Input Signal .....	2-38
2-47	Displaying Multiple Peaks .....	2-39
2-48	Displaying Relative Values .....	2-39
2-49	SNR .....	2-40
2-50	WDM Signal Connections .....	2-41
2-51	Measuring the Spectrum of a WDM Signal .....	2-42
2-52	WDM Monitor Screen .....	2-42
2-53	WDM Dialog Box Screen .....	2-43
2-54	WDM Monitor Measurement Screen .....	2-44
2-55	Displaying WDM Monitor SNR .....	2-45
2-56	Displaying WDM Monitor Level .....	2-45
2-57	Displaying WDM Monitor Relative Values (INITIAL) .....	2-46
2-58	Displaying WDM Monitor Relative Values (NOMINAL) .....	2-46
2-59	Displaying WDM Monitor Channels .....	2-47
2-60	Measuring the Reference Data Used for Filter Transmission Characteristics .....	2-48
2-61	Displaying the Limit Line .....	2-49
2-62	Connections Used for Device Evaluation .....	2-50
2-63	Transmission Characteristics of a Device to Be Evaluated (with the Limit Line Displayed) .....	2-50
2-64	Label Data .....	2-57
2-65	Selecting the Floppy Disk .....	2-64
5-1	Block Diagram .....	5-18
A-1	Typical Mach-Zehnder Interferometer Configuration .....	A-6

## LIST OF TABLES

No.	Title	Page
1-1	Standard Accessories List .....	1-2
1-2	Option .....	1-2
1-3	Accessories (Sold Separately) .....	1-2
1-4	Limited-life Part .....	1-2
1-5	Power Cable Options .....	1-3
1-6	Power Supply Specifications .....	1-5
2-1	Status Display Contents .....	2-10
2-2	Recommended Printers .....	2-62
3-1	Changing the Table Data Display and the Current Time or Channel .....	3-32
3-2	Default Settings .....	3-45
4-1	Interface Functions .....	4-4
4-2	Initial State After Turning the Power On .....	4-26
4-3	State Changes According to the Commands .....	4-27
4-4	FUNCTION (1 of 2) .....	4-29
4-6	LABEL .....	4-31
4-7	MEASURE .....	4-31
4-5	CURSOR .....	4-31
4-8	DISPLAY (1 of 5) .....	4-32
4-9	DATA OUT .....	4-37
4-10	Codes Corresponding to Other Keys .....	4-38
4-11	Controlling Data Output and Others (1 of 3) .....	4-38
4-12	Error Codes Associated with the Self-diagnosis Function .....	4-40
5-1	Throughput, Sensitivity and Dynamic Range for Each Measurement Mode at a Wavelength of 1.55 $\mu\text{m}$ (typical value) .....	5-2
5-2	Number of Signals and Interpolation Method. ....	5-9

## 1 INTRODUCTION

This chapter provides the following information:

- Product description
- A list of standard accessories and power cable options
- Operating environment
- How to verify that the spectrum analyzer is functioning properly
- How to set the print paper
- How to clean, store, and transport the spectrum analyzer

### 1.1 Product Overview

The Q8384 is an optical spectrum analyzer of the spread spectral method using the diffraction grating monochromator.

The features of the optical spectrum analyzer are as follows:

- (1) Performance compliant with optical communication devices such as EDFA, AWG and the fiber grating.
  - Wavelength resolution: 10 pm or higher
  - Wide dynamic range: 60 dB or more
  - High wavelength accuracy:  $\pm 20$  pm
  - Polarization dependency:  $\pm 0.05$  dB
- (2) WDM analysis function  
Using the EDFA analysis function (with WDM) and the relationships between wavelengths and levels are easily observed by displaying a list of wavelengths.
- (3) Optical connectors that can be replaced by the user  
Users can easily replace optical connector types FC, SC and ST.
- (4) Operability and a large-size color LCD  
Measurements are taken easier than earlier models by use of operability-minded panel key arrangement and soft menus. In addition, the display is now of an 8.4-inch high-intensity TFT color LCD to offer you more visibility.
- (5) Printer output  
A high-speed thermo-sensitive printer is equipped as standard to output the screen data. Furthermore, the optical spectrum analyzer is equipped with a port which is used for a printer format ESC/P, ESC/P-R or PCL.
- (6) 3.5-inch floppy disk drive  
This drive is used to save measurement data and set conditions. The measurement data is saved in text format. This data, however, can be saved in bitmap format as screen image so that you can analyze it or make reports on an external computer.



## 1.2 Accessories, Option and Limited-life Part

## 1.2 Accessories, Option and Limited-life Part

The standard accessories shipped with the spectrum analyzer are listed in Table 1-1. The option, the accessories separately sold, and the parts with limited-life are listed in Tables 1-2, 1-3 and 1-4, respectively. If any of the accessories are damaged or missing or, to order additional accessories, contact a sales representative.

## 1.2.1 Standard Accessories

Table 1-1 Standard Accessories List

Accessory Name	Model Number	Quantity	Remarks
Power cable	A01402	1	*1
Power fuse	EAWK3.15A	1	3.15A (including the fuse holder)
Print paper	A09075 *2	1	Thermal paper with 114 mm wide, 1 roll
3.5-inch floppy disk	---	1	2HD
Operation Manual	EQ8384	1	English version

\*1: The cable supplied with the optical spectrum analyzer depends on what type (specified by model number above) was ordered when the optical spectrum analyzer was purchased.

There are 11 types of power cable available (see Table 1-2).

To order another power cable, contact a sales representative. When ordering, refer to power cables by their option number or model number.

\*2: You can order in boxes (each box contains five rolls) by specifying this code.

## 1.2.2 Option and Accessories

Table 1-2 Option

Accessory Name	Model Number	Remarks
Light source used for calibration	Option 25	Factory option

Table 1-3 Accessories (Sold Separately)

Accessory Name	Model Number	Remarks
SC connector	A08162	Optical connector
ST connector	A08163	Optical connector
FC connector	A08161	Optical connector







## 1.2.3 Limited-life Part

The fan filter should be replaced when it becomes clogged with dirt and cannot be cleaned well, or when it is broken. If you need a replacement filter, contact your sales representative or the nearest ADVANTEST sales office.

Table 1-4 Limited-life Part

Accessory Name	Model Number	Remarks
Fan filter	YEE-002124	Comes with the plastic guard.

Table 1-5 Power Cable Options

Plug configuration	Standards	Rating, color and length	Model number (Option number)
	JIS: Japan Law on Electrical Appliances	125 V at 7 A Black 2 m (6 ft)	Straight: A01402 Angled: A01412
	UL: United States of America CSA: Canada	125 V at 7 A Black 2 m (6 ft)	Straight: A01403 (Option 95) Angled: A01413
	CEE: Europe DEMKO: Denmark NEMKO: Norway VDE: Germany KEMA: The Netherlands CEBEC: Belgium OVE: Austria FIMKO: Finland SEMKO: Sweden	250 V at 6 A Gray 2 m (6 ft)	Straight: A01404 (Option 96) Angled: A01414
	SEV: Switzerland	250 V at 6 A Gray 2 m (6 ft)	Straight: A01405 (Option 97) Angled: A01415
	SAA: Australia, New Zealand	250 V at 6 A Gray 2 m (6 ft)	Straight: A01406 (Option 98) Angled: -----
	BS: United Kingdom	250 V at 6 A Black 2 m (6 ft)	Straight: A01407 (Option 99) Angled: A01417

1.3 Operating Environment

1.3 Operating Environment

This section describes the environmental conditions and power requirements necessary to use the optical spectrum analyzer.

1.3.1 Environmental Conditions


The Q8384 should be only be used in an area which satisfies the following conditions:

- Ambient temperature: 10 °C to +40 °C (operating temperature)
- Relative humidity: 85% or less (without condensation)
- An area free from corrosive gas
- An area away from direct sunlight
- A dust-free area
- An area free from vibrations
- A low noise area


Although the Q8384 has been designed to withstand a certain amount of noise riding on the AC power line, it should be used in an area of low noise. Use a noise cut filter when ambient noise is unavoidable.

- Installation position


The Q8384 has an exhaust cooling fan on the rear panel. Never block the area of this fan since the resulting internal temperature rise will affect measurement accuracy. In addition, use this instrument in a horizontal position at a maximum angle of 10°, or the measurement may be inaccurate.

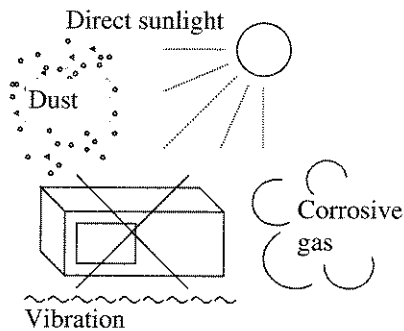


- Avoid operation in the following areas.

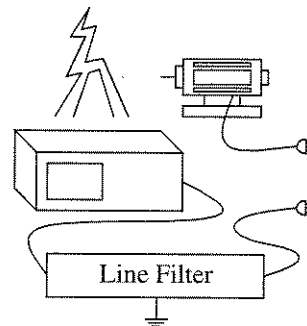

- Use a noise cut filter when there is a large amount of noise riding on the power line.



- Do not use the analyzer upright turned the rear panel side down.

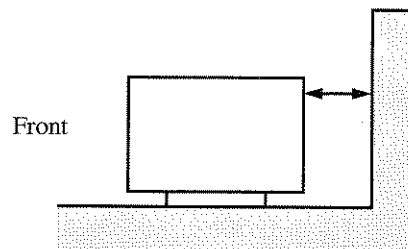

- Keep the rear panel 10 centimeters away from the wall

Figure 1-1 Operating Environment

The Q8384 can be used safely under the following conditions:

- Altitude: 2000 m maximum above the sea level
- Installation category II
- Pollution degree 2

### 1.3.2 Power Requirements

The power supply specifications of the optical spectrum analyzer are listed in Table 1-3.

**Table 1-6 Power Supply Specifications**

	100 VAC Operation	200 VAC Operation	Remarks
Input voltage range	90 V to 132 V	198 V to 250 V	Automatically switches between input levels of 100 VAC and 200 VAC.
Frequency range	48 Hz to 66 Hz		
Power consumption	220 VA or below		

---

**CAUTION:** *To prevent damage, operate the optical spectrum analyzer within the specified input voltage and frequency ranges.*

---

1.3.3 Power Fuse

### 1.3.3 Power Fuse

The power fuse is placed in the fuse holder which is mounted on the rear panel. A spare fuse is located in the fuse holder.

To check or replace the power fuse, use the following procedure:

1. Press the **POWER** switch to the OFF position.
2. Disconnect the power cable from the AC power supply.
3. Remove the fuse holder on the rear panel.
4. Check (and replace if necessary) the power fuse and put it back in the fuse holder.

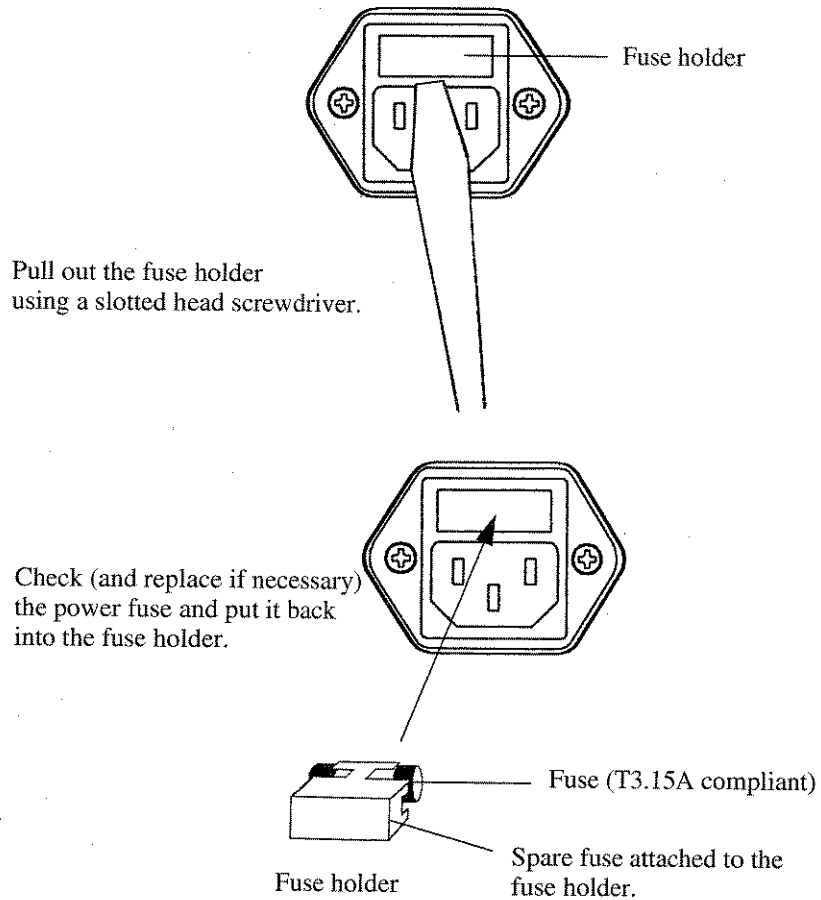


Figure 1-2 Replacing the Power Fuse

### 1.3.4 Power Cable

---

**CAUTION:**

1. Use a power cable rated for the voltage in question. Be sure however to use a power cable conforming to safety standards of your nation when using a product overseas (See Table 1-2).
  2. Be sure to plug the power cable into an electrical outlet which has a safety ground terminal. Grounding will be defeated if you use an extension cord which dose not include a safety ground terminal.
  3. Turn the **POWER** switch (on the front panel) off prior to connecting the power cable.
- 

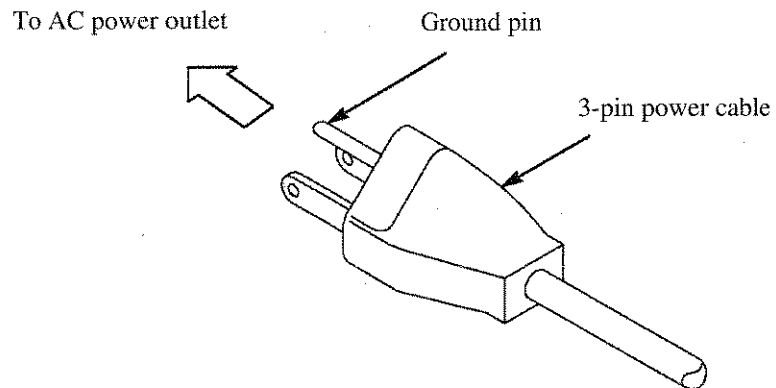


Figure 1-3 Power Cable

## 1.4 System Checkout

### 1.4 System Checkout

This section describes the Self Test which must be performed when operating the optical spectrum analyzer for the first time. Follow the procedure below:

1. Make sure that the **POWER** switch on the front panel is in the OFF position.
2. Connect the power cable provided to the AC power supply connector on the rear panel.

---

**CAUTION:** *To prevent damage, operate the optical spectrum analyzer within specified input voltage and frequency ranges.*

---

3. Connect the power cable to the outlet.
4. Press the **POWER** switch to the ON position.  
The Q8384 performs the self-diagnostics for a few seconds. When the self-diagnostics is complete, the self-test is then automatically started and the results will be displayed in sequence.

---

**CAUTION:** *Contact ADVANTEST for repair when the self test fails. Refer to the addresses at the end of this manual.*

---

The initial checkout is now complete, and the measurement screen is displayed.

## 1.5 Setting the Print Paper

Mount the paper in the internal printer as illustrated on the rear of the printer cover.


### Procedure

1. Set the head up lever to the open position.
2. Load the roll paper in the holder with the outside of the paper roll down.
3. Set up the paper as shown in the following figure.

---

**NOTE:** Be sure to insert the paper from the upper slit. The printer does not operate even if the paper is inserted into the lower slit.

---

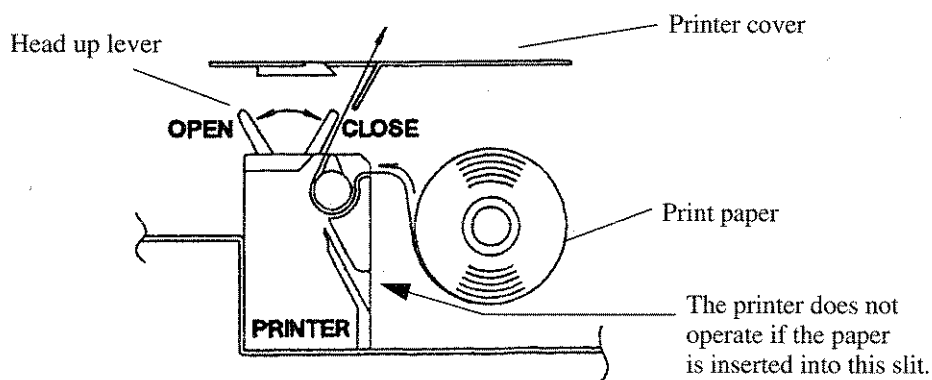

**Figure 1-4 Setting the Print Paper**

4. Set the head up lever to the close position.
5. Press the **FEED** key on the front panel and check whether the paper is correctly installed. Return to the step 1 if the paper is not correctly installed.

Printer paper: A09075 (Order No.)  
 5 rolls/box (Order unit: 1 box)  
 Thermosensitive paper length : 30 m  
 Paper width : 114 mm

---

**CAUTION:** Use only the specified paper.

---



## 1.6 Cleaning, Storing and Transporting the Q8384 Optical Spectrum Analyzer

### 1.6.1 Cleaning

Remove dust from the outside of the optical spectrum analyzer by wiping or brushing the surface with a soft cloth or small brush. Use a brush to remove dust from around the panel keys. Hardened dirt can be removed by using a cloth which has been dampened in water containing a mild detergent.

---

**CAUTION:**

1. Do not allow water to get inside the optical spectrum analyzer.
  2. Do not use organic cleaning solvents, such as benzene, toluene, xylene, acetone or similar compounds, since these solvents may damage the plastic parts.
  3. Do not use abrasive cleaners.
- 

- Cleaning the Display Filter

Normally cleaning the display filter from the front should be sufficient. However, if necessary, the filter itself can be detached from the optical spectrum analyzer by removing the two screws on the front. Clean the backside of the filter with a soft cloth.

---

**CAUTION:** Do not touch the LCD display with your finger when the filter has been removed.

---

- Cleaning the optical input connectors

The optical input section of the Q8384 is easy to clean because of the replaceable adapter used. The optical input section is accessible when you remove the adapter. Clean the tip with alcohol.

---

**NOTE:** Measurement may be inaccurate when the instrument is used with the input section dirty.

---

- Cleaning the fan filter

The fan filter collects dirt particles from the air over time. When the filter gets dirty, remove the plastic guard and remove the dirt from the filter by hand.

### 1.6.2 Storing

Store the optical spectrum analyzer in an area which has a temperature from -10 °C to +50 °C. If you plan to store the optical spectrum analyzer for a long period (more than 90 days), put the optical spectrum analyzer in a vapor-barrier bag with a drying agent and store the optical spectrum analyzer in a dust-free location out of direct sunlight.

### 1.6.3 Replacing and Cleaning the Optical-Connector Adapter of Q8384

(1) Replacing the Optical-connector Adapter

The FC-type connector adapter is equipped with standard for the Q8384. The optional optical-connector adapters such as SC-type or ST-type are provided as accessories. The method of replacing the optical-connector adapter is shown in Figure 1-5. Easy replacement can be conducted by removing the fixed cap for the adapter and pulling out the adapter.

(2) Cleaning the Optical Connector

Remove the adapter same as the procedure of adapter replacement and clean the tip of light-input/output sections with alcohol. If the Q8384 are used with the dirty light-input/output parts, some error may occur in its measurement value.

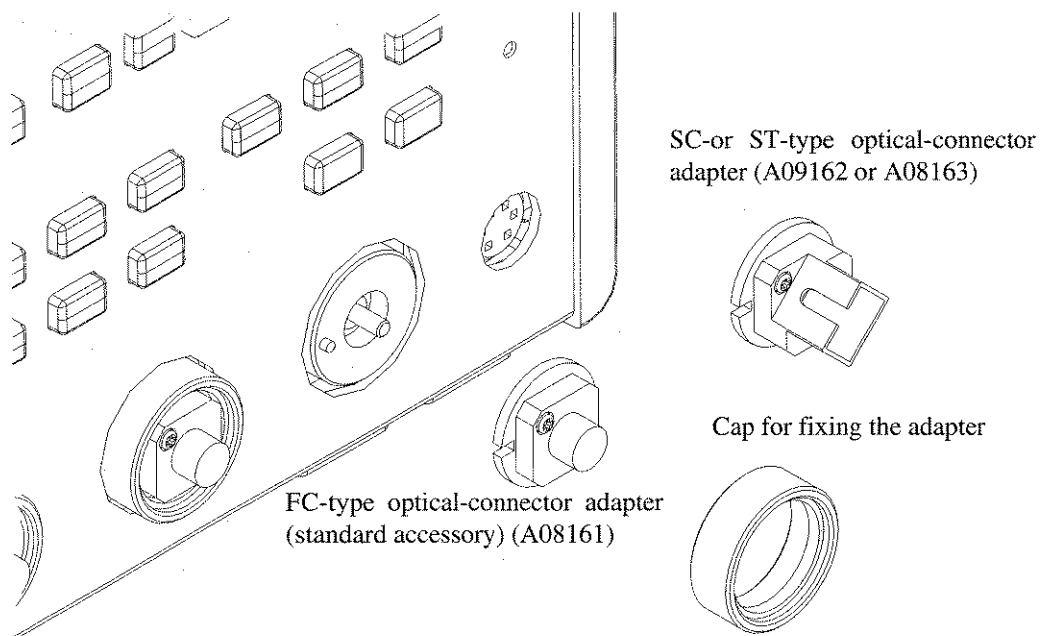


Figure 1-5 Replacing and Cleaning the Optical-connector Adapter

**NOTE:**

1. *Screw up surely after clearing of the optical connector and or exchanging of the optical connector adapter.*
2. *The optical connector adapter used in the optical spectrum analyzer uses a sleeve made of zirconia that is extremely durable. However, make sure that you insert the optical connector correctly or you do not pry it out to avoid bending or damaging the sleeve.*

## 1.6.4 Transporting

### 1.6.4 Transporting

When you ship the optical spectrum analyzer, use the original container and packing material. If the original packaging is not available, pack the optical spectrum analyzer using the following guidelines:

- To allow for cushioning, use a corrugated cardboard container with inner dimensions that are at least 15 centimeters more than those of the optical spectrum analyzer.
- Surround the optical spectrum analyzer with plastic sheeting to protect the finish.
- Cushion the optical spectrum analyzer on all sides with packing material or plastic foam.
- Seal the container with shipping tape or a heavy-duty, industrial stapler.
- Be careful when carrying the optical spectrum analyzer because it is a heavy instrument.

If you are shipping the optical spectrum analyzer to a service center for service or repair, attach a tag to the optical spectrum analyzer that shows the following information:

- Owner and address
- Name of a contact person at your location
- Serial number of the optical spectrum analyzer (located on the rear panel) Description of the service requested

### 1.7 Warm-up time

A warm-up time of 30 minutes is required to guarantee the specified accuracy.

### 1.8 About Calibration

When you want to calibrate the Q8384, please contact a sales representative.

Desirable Period	One year
------------------	----------

## 2 OPERATION

This chapter describes the following.

- Description on the front and rear panels
- Screen annotation
- Basic operation
- Measurement examples
- Expanded functions

### 2.1 Panel Description

This section describes the names, functions and screen annotations of the front and rear panels.

#### 2.1.1 Front Panel

The panel keys and connectors are described below for each section of the front panel.

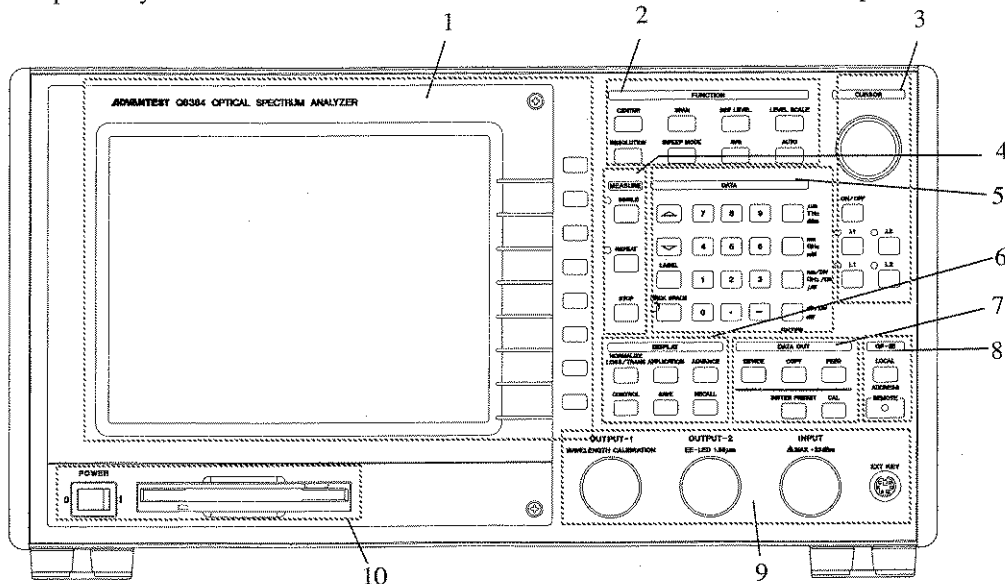


Figure 2-1 Front Panel

The front panel consists of 10 sections as shown below.

1. LCD Display Section
2. FUNCTION Section
3. CURSOR Section
4. MEASURE Section
5. DATA Section
6. DISPLAY Section
7. DATA OUT Section
8. GP-IB Section
9. Connector Section
10. POWER Switch/Floppy Disk Drive Section

2.1.1 Front Panel

2.1.1.1 LCD Display Section

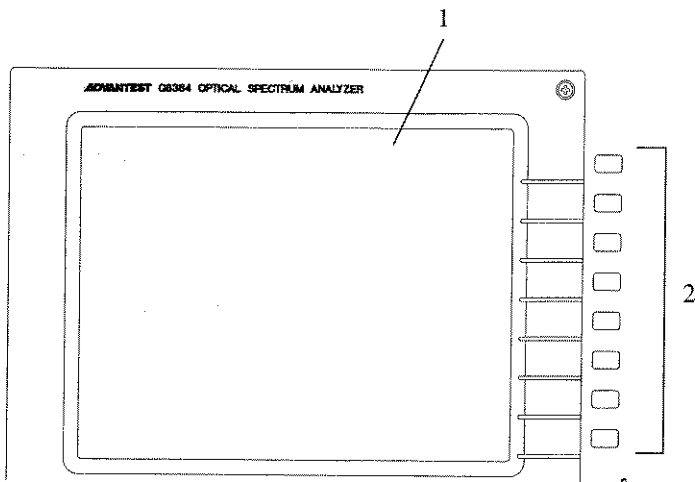


Figure 2-2 LCD Display Section

- |                                 |   |
|---------------------------------|---|
| 1. Liquid crystal display (LCD) | Displays trace and measured data.   |
| 2. Soft keys                    | Eight keys corresponding to the soft-menu display on the left; pressing a soft key selects the corresponding menu item. |

## 2.1.1.2 FUNCTION Section

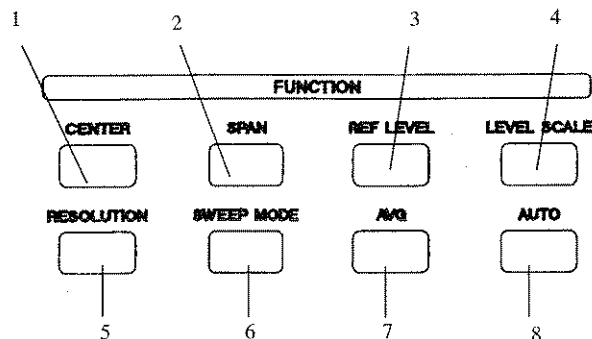


Figure 2-3 FUNCTION Section

- |                           |  |
|---------------------------|--|
| 1. <b>CENTER</b> key      | Specifies the center wavelength or center frequency to be analyzed.  |
| 2. <b>SPAN</b> key        | Specifies the wavelength span or frequency span to be analyzed, and the start and stop wavelengths or frequencies. |
| 3. <b>REF LEVEL</b> key   | Specifies the reference level in display.  |
| 4. <b>LEVEL SCALE</b> key | Selects the level axis (LIN/LOG) and specifies the scale.  |
| 5. <b>RESOLUTION</b> key  | Specifies the wavelength resolution.   |
| 6. <b>SWEEP MODE</b> key  | Specifies the sweep mode correspond to the input signal.   |
| 7. <b>AVG</b> key         | Specifies the number of times averaging or smoothing is performed.   |
| 8. <b>AUTO</b> key        | Executes the automatic setting functions for most suitable wavelength/level.                                       |

2.1.1 Front Panel

2.1.1.3 CURSOR Section

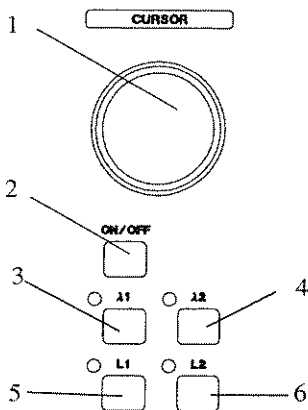


Figure 2-4 CURSOR Section

- |    |                   |  |
|----|-------------------|--|
| 1. | Data knob         | Moves the cursor selected and continuously changes the data set. |
| 2. | <b>ON/OFF</b> key | Controls ON/OFF of all cursors and the cursor display mode.      |
| 3. | <b>λ1</b> key     | Selects display and erases wavelength cursor 1.                  |
| 4. | <b>λ2</b> key     | Selects display and erases wavelength cursor 2.                  |
| 5. | <b>L1</b> key     | Selects display and erases level cursor 1.                       |
| 6. | <b>L2</b> key     | Selects display and erases level cursor 2.                       |

2.1.1.4 MEASURE Section

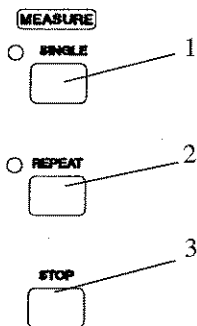


Figure 2-5 MEASURE Section

- |    |                   |                             |
|----|-------------------|-----------------------------|
| 1. | <b>SINGLE</b> key | Executes one time sweeping. |
| 2. | <b>REPEAT</b> key | Repeats sweeping.           |
| 3. | <b>STOP</b> key   | Stops sweeping.             |

## 2.1.1.5 DATA Section

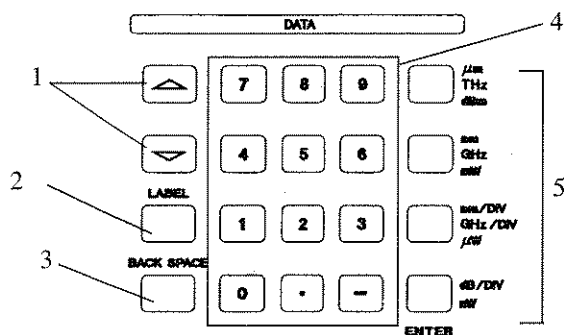


Figure 2-6 DATA Section

- |    |                               |   |
|----|-------------------------------|---|
| 1. | Step keys                     | Used to move the cursor selected and change the data set, step by step.   |
| 2. | <b>LABEL</b> key              | Specifies the label data.   |
| 3. | <b>BACK SPACE</b> key         | Deletes a character from the input data.  |
| 4. | Numeric keys                  | Used to enter numeric values.<br>There are ten number keys (0 through 9), a decimal point key (.) and a minus key (-).  |
| 5. | Units keys ( <b>ENTER</b> key | <p><b>μm, THz, dBm</b> key<br/>Sets μm, THz or dBm.</p> <p><b>nm, GHz, mW</b> key<br/>Sets nm, GHz or mW.</p> <p><b>nm/DIV, GHz/DIV, μW</b> key<br/>Sets nm/DIV, GHz/DIV or μW.</p> <p><b>dB/DIV, nW</b> key<br/>Sets dB/DIV or nW.</p> |

This key is also used to confirm data.

When you attempt to enter other dimensional or numeric values, the unit keys can be used as ENTER keys.



2.1.1 Front Panel

2.1.1.6 DISPLAY Section

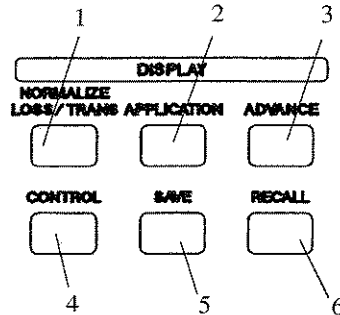


Figure 2-7 DISPLAY Section

1. **NORMALIZE LOSS/TRANS** key Executes measurement data normalization and measurement of loss and transparency characteristics.
2. **APPLICATION** key Used for calculating the spectral width, notch width, and the gain and noise figure for the EDFA (Erbium-Doped Fiber Amplifier) as well as for setting the WDM Analysis.
3. **ADVANCE** key Executes a peak power monitor or limit line measurement.
4. **CONTROL** key Specifies the display mode (superimpose, dual-screens).
5. **SAVE** key Used to save measurement data.
6. **RECALL** key Used to recall set measurement data previously saved.

### 2.1.1.7 DATA OUT Section

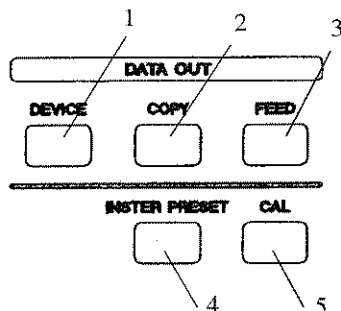


Figure 2-8 DATA OUT Section

- |                            |   |
|----------------------------|---|
| 1. <b>DEVICE</b> key       | Specifies a device (printer, floppy disk, clock or buzzer). |
| 2. <b>COPY</b> key         | Executes data out processing.                               |
| 3. <b>FEED</b> key         | Feeds paper to the printer.                                 |
| 4. <b>INSTR PRESET</b> key | Initializes the setting modes.                              |
| 5. <b>CAL</b> key          | Calibrates the wavelength and the level.                    |

### 2.1.1.8 GP-IB Section




Figure 2-9 GP-IB Section

- |                       |  |
|-----------------------|--|
| 1. <b>LOCAL</b> key   | Specifies the local mode to make the panel keys valid (when the REMOTE lamp is lit). |
| <b>ADDRESS</b> key    | Specifies the GP-IB address (when the REMOTE lamp is off).                           |
| 2. <b>REMOTE</b> lamp | Lit when in the remote state.  |

2.1.1 Front Panel

2.1.1.9 Connector Section

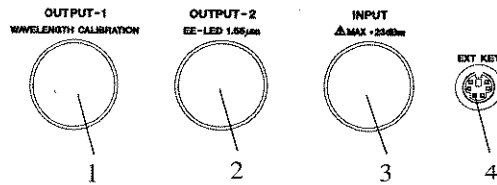


Figure 2-10 Connector Section

- |                              |   |
|------------------------------|---|
| 1. <b>OUTPUT-1</b> connector | Used to output the optical signal from a calibration light source (Option). To automatically measure the wavelength, connect the optical fiber from the OUTPUT-1 connector to the INPUT connector.  |
| 2. <b>OUTPUT-2</b> connector | Used to output the optical signal from a EE-LED light source (Option).  |
| 3. <b>INPUT</b> connector    | Used to input the light source to be measured.  |
| 4. <b>EXT KEY</b> connector  | Used to connect a PS/2 type (MiniDIN6 pins) keyboard. The external keyboard is used to enter label names and file names. Be sure to use a keyboard with a connector which includes a built-in ferrite core. We recommend the following keyboards:<br>Japanese layout, 109 key: Fujitsu FKB-8724-501<br>US layout, 104 key: Fujitsu FKB-8725-401 |

**CAUTION:** To prevent damage, never attempt to apply an input whose total power is +23 dBm or more to the INPUT terminal on the optical spectrum analyzer. In addition, never attempt to apply an external optical output to the OUTPUT-1 and OUTPUT-2 terminals on the optical spectrum analyzer.

2.1.1.10 POWER Switch/Floppy Disk Drive Section

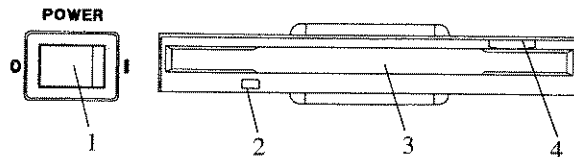


Figure 2-11 POWER Switch and Floppy Disk Drive Section

- |                           |   |
|---------------------------|---|
| 1. <b>POWER</b> switch    | Turns power ON/OFF.   |
| 2. Eject button           | Used to eject floppy disks from the drive.                    |
| 3. Floppy disk drive door | Insert floppy disks here.                                     |
| 4. Access lamp            | Turns on when the floppy disk in the drive is being accessed. |

## 2.1.2 Screen Annotation

This section describes typical screen annotations using the power monitor as an example.

### (1) Screen Annotation

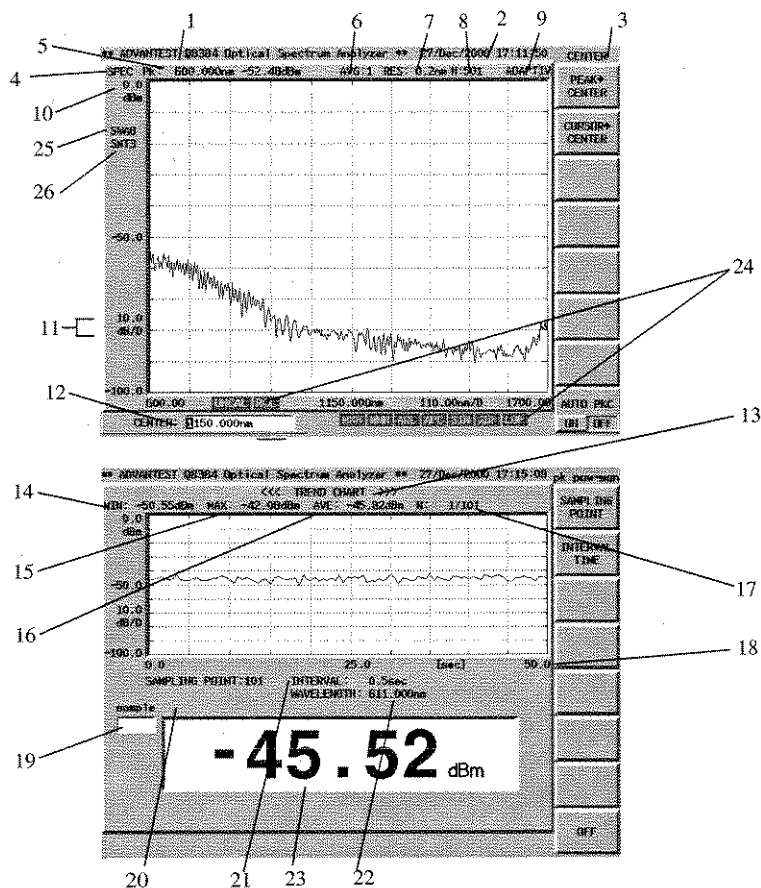


Figure 2-12 Screen Annotation

- |                             |  |
|-----------------------------|--|
| 1. Label display            | 14. Measured minimum value   |
| 2. Date                     | 15. Measured maximum value   |
| 3. Soft key type            | 16. Measured average value   |
| 4. Analysis data type       | 17. Measured points  |
| 5. Peak search data display | 18. Measurement time   |
| 6. Number of point averages | 19. Sampling indicator   |
| 7. Resolution               | 20. Measurement count setting value                                      |
| 8. Sampling points          | 21. Measurement time interval setting value                              |
| 9. Sweep mode               | 22. Wavelength at the current peak                                       |
| 10. REF level display       | 23. Power display  |
| 11. 1 scale of vertical     | 24. Status display   |
| 12. Input window            | 25. Number of sweep averages, or a trace number when set to multi-trace. |
| 13. Analysis data type      | 26. Number of smoothing points   |

## 2.1.2 Screen Annotation

Table 2-1 Status Display Contents

Display	Description
UNCAL	This warning is displayed when the sweep width along the wavelength is smaller than the wavelength specified by the wavelength resolution at a measurement point. When measuring a line spectrum under the following condition, the level displayed is lower than the actual level because the peak level cannot be detected correctly: Wavelength resolution [nm] $\times$ (Number of sampling points - 1) < Span [nm]
RCL	Indicates that the waveform was loaded from memory or from a floppy disk.
MXH	The MAX HOLD function is turned on.
MNH	The MIN HOLD function is turned on.
ARL	The auto-reference level function is turned on.
APC	The auto-peak center function is turned on.
SIM	The superimposing function is turned on.
$\lambda$ OF	The wavelength offset function is turned on while an offset other than 0 is being input.
LOF	The level offset function is turned on while an offset other than 0 is being input.

### 2.1.3 Rear Panel

This subsection shows the rear panel and describes its terminals and connectors.

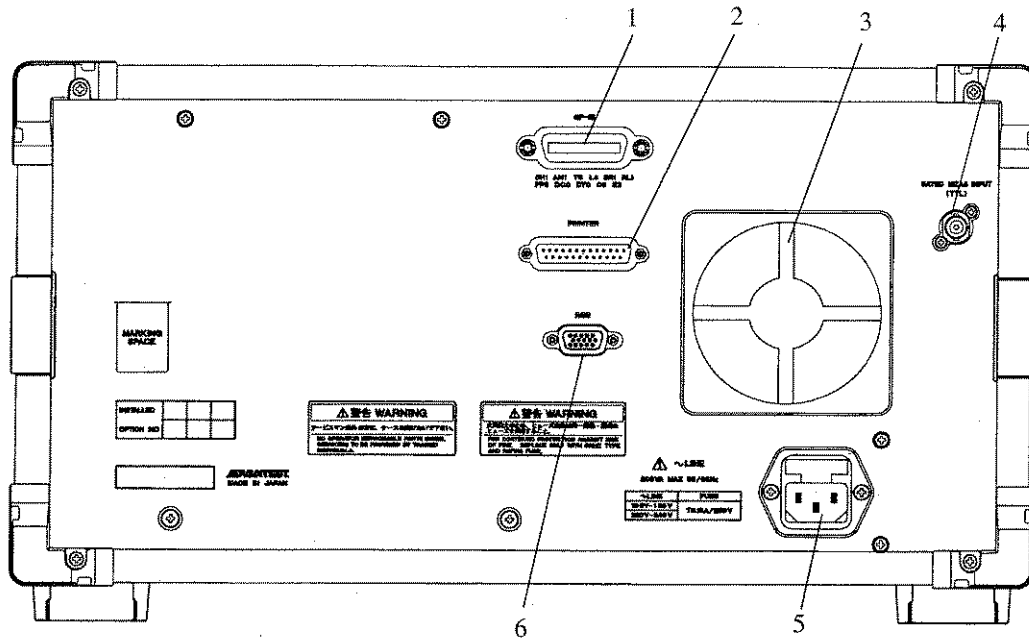


Figure 2-13 Rear Panel

- |   |  |
|---|--|
| 1. <b>GP-IB</b> connector                               | Connector for an external controller used when set to remote control through GPIB interface.                 |
| 2. <b>PRINTER</b> connector                             | Connector for a printer  |
| 3. Fan  | Cooling fan  |
| <hr/> <b>CAUTION:</b> Do not block the air vents. <hr/> |  |
| 4. <b>GATED MEAS INPUT</b> connector                    | Connector to input a signal used for the gated measurement in sync with the TTL-level positive pulse signal. |
| 5. AC power connector                                   | Connect the input power cable from the analyzer to the outlet of the AC power source.                        |
| 6. <b>RGB</b> connector                                 | Connector for an external monitor compatible with VGA specifications.  |

## 2.2 Basic Operation

This section describes the method of how to go through the menus and use the measurement functions.

### 2.2.1 Operating Menus and Entering Data

This section explains how the panel keys and soft keys are used.

#### (1) Selecting the menu

If you press a panel key, the soft menu associated with that key is displayed in the soft menu area on the screen.

To set measurement conditions, press a panel key to select the soft menu you wish.

To make a soft menu selection, press the soft key next to the menu item.

Once the soft menu is displayed, the titles of the set items and their current settings are displayed in the area outside the trace display section.

In addition, if there is an associated menus are also displayed (Refer to (3) Soft menu configuration).

For the items which require alphanumeric characters, the input window is displayed.

For example, the following screen will be displayed when you press **CENTER**.

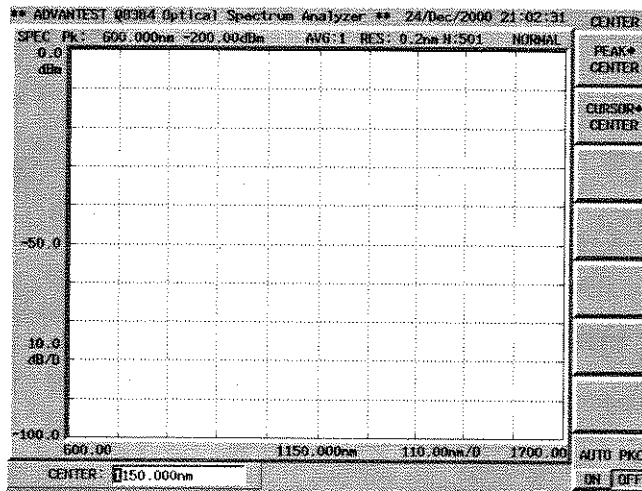


Figure 2-14 CENTER Menu

#### (2) Entering data

The data in the input window can be changed using the numeric keys, step keys or data knob while the window is displayed.

- Entering data using the numeric keys

You use the following keys to enter data: the numeric keys or the **BACK SPACE**. If you make a mistake when using the numeric keys, you can use the **BACK SPACE** key to delete the last digit entered. After entering the data, pressing one of the other unit keys completes the operation.

---

**CAUTION:** *Data entered with the numeric keys that is not terminated with a units terminator is aborted when you press any panel key.*

---

Example 1: The following example sets the reference level to -20 dBm using the numeric keys:  
Press **REF LEVEL**, **-**, **2**, **0** and **dBm**.

- Entering data using the step keys

The step keys are used to enter data in a predefined step size. Press the  $\nabla$  step key to decrease the value and the  $\Delta$  step key to increase the value. You can enter data while looking at the input window and the trace on the screen using the step keys. The step sizes vary depending on the items to be set.

Example 2: The following example sets the reference level to 0 dBm using the step keys:

Press the  $\Delta$  step key following Example 1. This sets the reference level to -15 dBm. This is available when the level scale is set to 10 dB/div.

Pressing the  $\Delta$  step key three times sets the reference level to 0.0 dBm.

- Entering data using the data knob

The data knob is used to set data in increments smaller than the step size. This is convenient when making fine adjustments to data already entered.

Example 3: The following example sets the reference level to 10 dBm using the data knob.

Turning the data knob clockwise increases the reference level in increments of 5 dB. Continue to turn it until the active area shows a setting of 10 dBm. This is available when the level scale is set to 10 dB/div.

Turning the data knob counter clockwise decreases the reference level by 5 dB.

- Removing the input window

To remove the input window, press the appropriate panel key again.

Example: Press the **CENTER** key. (The input window is displayed.)

Press the **CENTER** key again. (The input window is removed.)

(3) Soft menu configuration

- Switching between settings on a toggle button

Press the soft key under the soft menu with switching capability to toggle between settings for ON/OFF, LIN/LOG and similar switches each time you press the soft key.

- Main menu and sub menu

Menus consist of the main menu and associated submenus. When **PREVIOUS MENU** is selected in the submenu, the screen display returns to the main menu.

If **OFF** is selected in the submenu, the current function is disabled and the screen display returns to the main menu.

In addition, there are some soft keys with which you can switch the setting each time you press them.

- Submenu

When a submenu item is displayed in lower-case characters, this indicates that there is another submenu: pressing this key again displays next level.



2.2.2 Light Spectrum Measurement

2.2.2 Light Spectrum Measurement

This section explains how to take a light source measurement for a 1.55 $\mu$ m multi mode laser diode as an example of a typical measurement.

Power on

---

**NOTE:** To take accurate measurements, use the analyzer within the specified temperature range, and wait at least 30 minutes after turning on the power before performing the Calibrations. In this exercise example, the warm-up and calibration are omitted.

---

1. Check to see if the **POWER** switch (on the front panel) is turned off.
2. Connect the power cable provided to the AC power supply connector on the rear panel.

---

**CAUTION:** To avoid damage to the analyzer, operate the analyzer within the specified input voltage and frequency ranges.

---

3. Connect the power cable to the outlet.
4. Turn on the **POWER** switch (on the front panel).  
When the self-diagnostics has completed, the self-test is started.

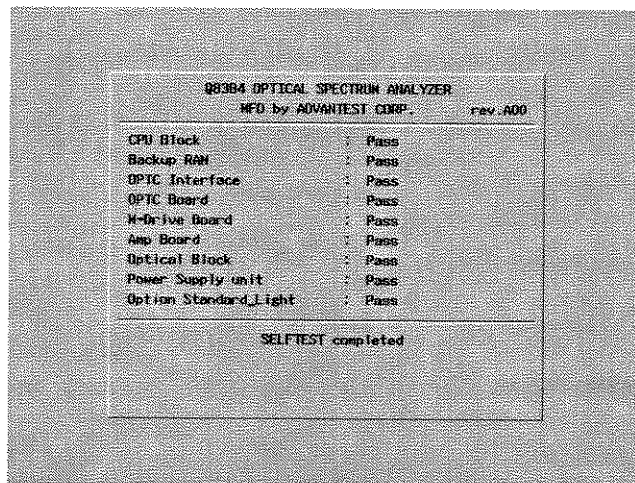


Figure 2-15 Self-test Screen

When the self-test has completed, the measurement screen is displayed

---

**NOTE:** The screen displayed after the power is turned on may differ from the one shown here depending on the current settings.

---

## Initialization

This resets the current settings to the initial settings.

1. Press **INSTR PRESET**.  
The INSTR PRESET menu is displayed.

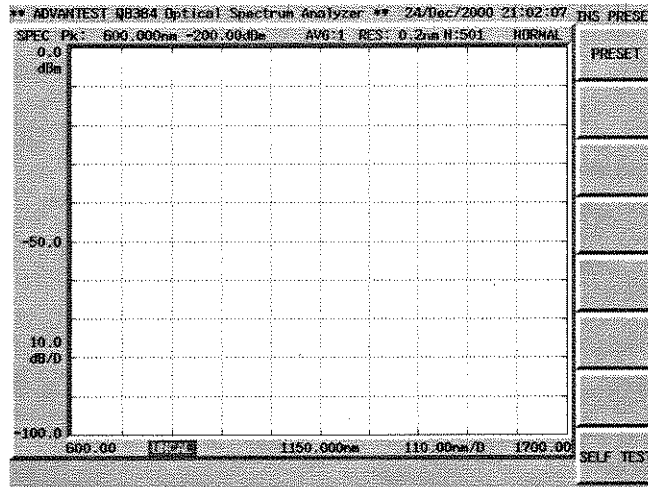


Figure 2-16 INSTR PRESET Menu

2. Press **PRESET**.  
The initial settings are displayed.

## Setup

Connect the light signal to the optical spectrum analyzer.

3. Connect the optical fiber cable from the output connector of light source to the optical spectrum analyzer **INPUT** connector.

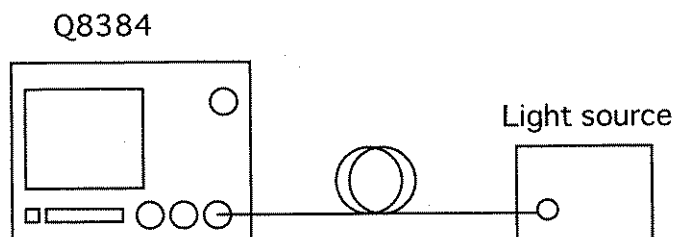


Figure 2-17 Light Spectrum Measurement

2.2.2 Light Spectrum Measurement

Setting the measurement conditions

This changes the analyzer settings so that the input signal is displayed more clearly.

4. Press **CENTER**.  
An input window is displayed.

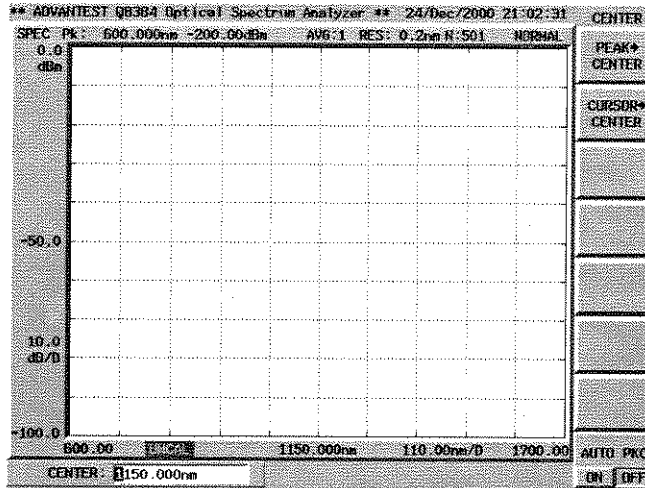


Figure 2-18 Input Window

5. Press **1**, **.**, **5**, **5** and **μm**.  
A center wavelength of 1.55 μm is set.

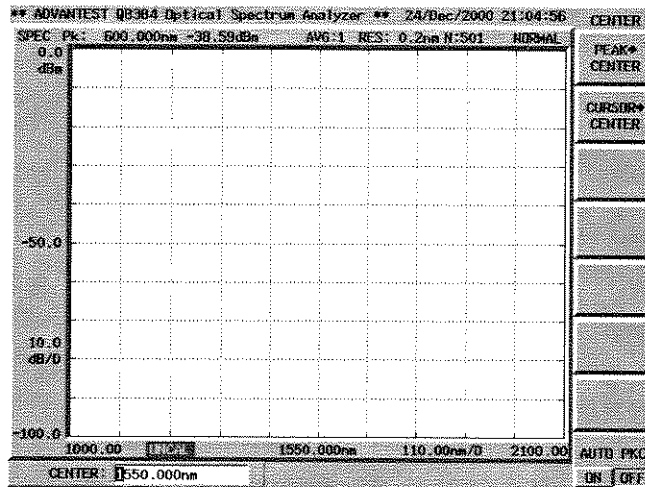


Figure 2-19 Setting the Center Wavelength

6. Press **SPAN**, **2**, **0** and **nm**.  
An analysis span of 20 nm is set.
7. Press **REF LEVEL**, **-**, **1**, **0** and **dBm**.  
The reference level is set to -10 dBm.

---

**NOTE:** The reference level is to specify the displaying level and does not affect measurement data. An optimum view is obtained by changing the reference level after a measurement has been taken.

---

8. Press **RESOLUTION**, **0**, **.**, **1** and **nm**.  
A resolution of 0.1 nm is set.

---

**CAUTION:** If a line spectrum is measured when the following condition applies, the level displayed is lower than the actual level because the peak level cannot be detected correctly:  
 $\text{Resolution} \times (\text{Number of sampling points} - 1) < \text{Span}$   
 The status of **uncal** is displayed on the screen when the above condition is satisfied.

---

#### Performing the measurement

9. Press **SINGLE**.  
A measurement is performed and the spectrum is displayed.

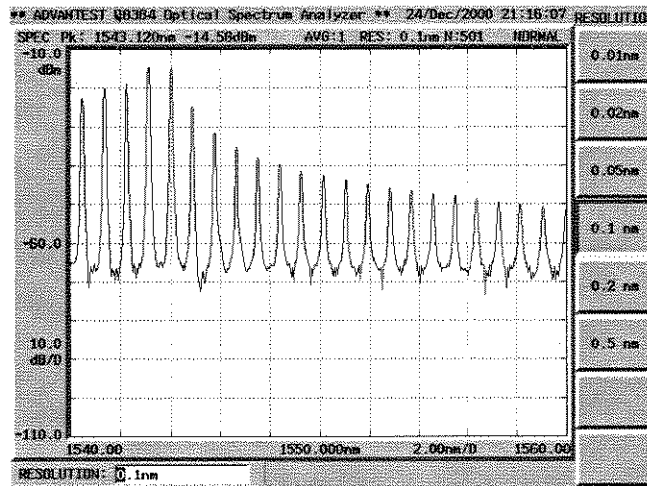


Figure 2-20 Displaying the Spectrum

#### Displaying the cursor

Data is read using the cursor.

10. Press **ON/OFF(ON)**.  
The cursor is displayed at the maximum peak and the wavelength of 1543.12 nm and the level of -14.58 dBm at the cursor position are displayed in the cursor area.

2.2.2 Light Spectrum Measurement

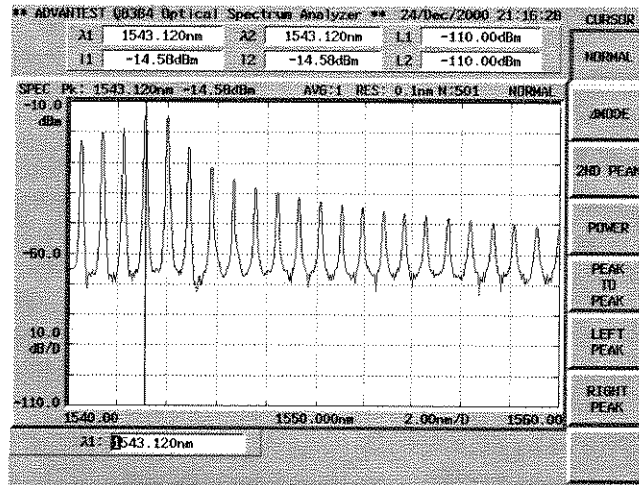


Figure 2-21 Peak Search

Changing the center wavelength

The highest peak can be displayed in the center of the screen using the following procedure.

11. **CENTER** and **PEAK**→**CENTER**.  
The peak wavelength becomes the center wavelength.  
(The cursor position stays unchanged.)

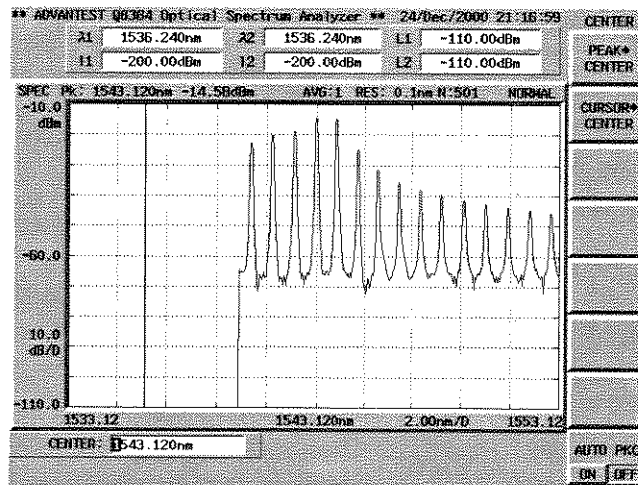


Figure 2-22 Changing the Center Wavelength

## Setting the analysis span

A special span in the spectrum is specified as the analysis span.

12. Press **ON/OFF(ON)** three times.
  - First time: The soft key menu changes to the **CURSOR** menu.
  - Second time: The cursor disappears.
  - Third time: A cursor is set to the peak.

X1 Cursor has been made active.

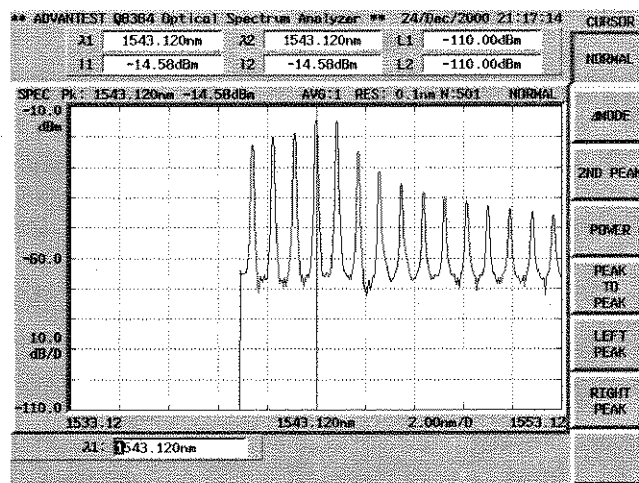


Figure 2-23 Displaying the Cursor

13. Turn the data knob to move the X1 cursor to the left end of the span you wish to analyze.
14. Press **λ2** and turn the data knob to move the X2 cursor to the right end of the span you wish to analyze.

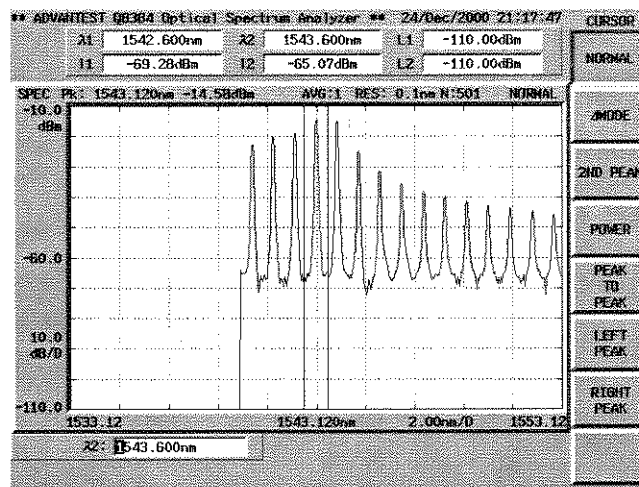


Figure 2-24 Setting the Analysis Span

2.2.2 Light Spectrum Measurement

15. Press **SPAN** and **CURSOR SPAN**.  
The span between the two X cursors becomes the analysis span.

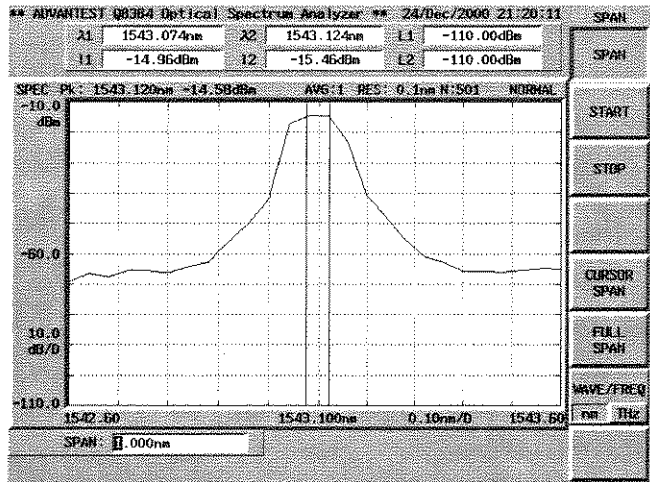


Figure 2-25 Setting the Analysis Span-1

Because only part of the span is selected, only a few measurements are used for analysis. However, the auto-panning and auto-zooming functions are used to interpolate the measurements to change the number of measurements to the number of specified sampling points and display the interpolated measurements.

16. Press **RESOLUTION**, **0**, **.**, **0**, **1** and **nm**.  
The resolution is set to 0.01 nm.
17. Press **SINGLE**.  
A sweep is carried out and the spectrum is displayed.

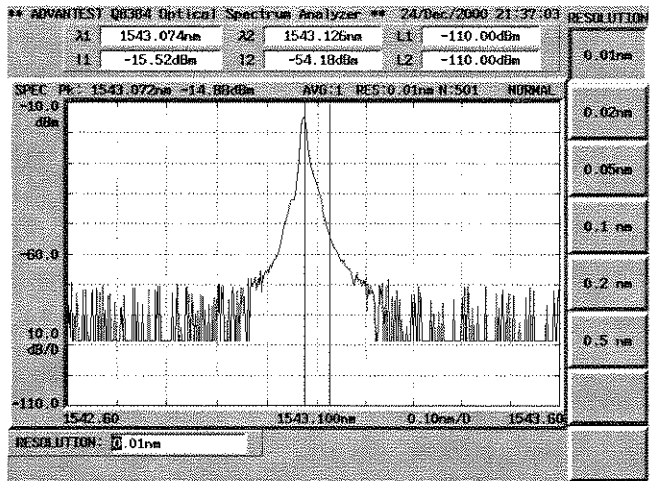


Figure 2-26 Setting the Analysis Span-2

To acquire data which is equivalent to the number of sample points specified, measurement is performed within the range specified by the X cursors. For more information on how to set the measurement conditions, refer to Section 2.2.11.

### 2.2.3 Peak Power Monitor Measurement

This section describes the peak power monitor function of the optical spectrum analyzer using a light source measurement of 1.55  $\mu\text{m}$  multi mode laser diode as an example.

#### Power on

1. Turn the **POWER** switch (on the front panel) on.  
The startup screen is displayed after the self-test has been completed.

#### Initialization

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The initial settings are displayed.

#### Setup

Connect the light signal to the optical spectrum analyzer.

3. Connect the optical fiber cable from the light source output connector to the optical spectrum analyzer INPUT connector.

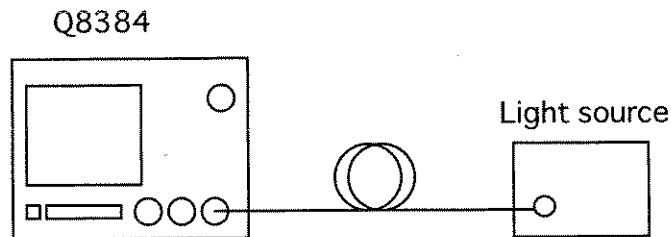


Figure 2-27 Peak Power Monitor Measurement

#### Setting the measurement conditions

This changes the analyzer settings so that the input signal is displayed more clearly.

4. Press **CENTER**, **1**, **.**, **5**, **5** and  **$\mu\text{m}$** .  
A center wavelength of 1.55  $\mu\text{m}$  is set.
5. Press **SPAN**, **2**, **0** and **nm**.  
An analysis span of 20 nm is set.
6. Press **REF LEVEL**, **-**, **1**, **0** and **dBm**.  
The reference level is set to -10 dBm.
7. Press **RESOLUTION**, **0**, **.**, **1** and **nm**.  
A resolution of 0.1 nm is set.



2.2.3 Peak Power Monitor Measurement

8. Press **SINGLE**.  
A sweep is performed and the resulting spectrum is displayed.

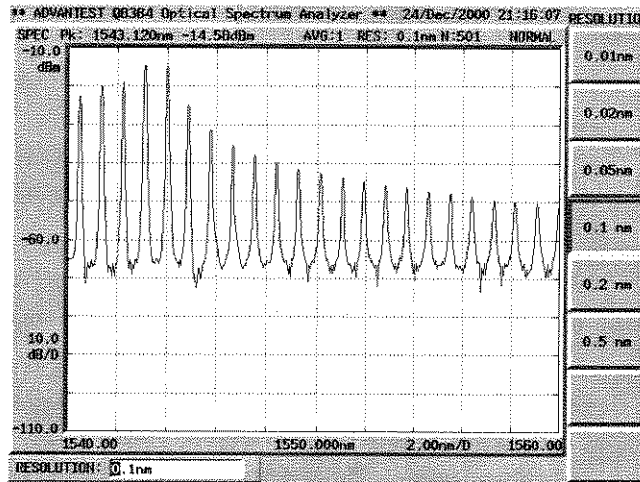


Figure 2-28 Displaying the Spectrum

Starting the peak power monitor

The targeted peak is displayed in the center of the screen.

1. Press **CENTER** and **PEAK→CENTER**.  
The peak wavelength becomes the center wavelength.  
The peak power monitor uses the previous conditions made before toggling the peak power monitor to ON.
2. Press **ADVANCE** and **peak power-mon**.  
The screen display is changed to the peak power monitor.
3. Press **INTERVAL TIME, 1** and **ENTER**.  
Time-varying characteristic is measured in increments of 1 seconds.
4. Press **SAMPLING POINT, 5, 1** and **ENTER**.  
Sets the optical spectrum analyzer to perform the measurement 51 times.
5. Press **SINGLE**.  
Starts the peak power monitor measurement.

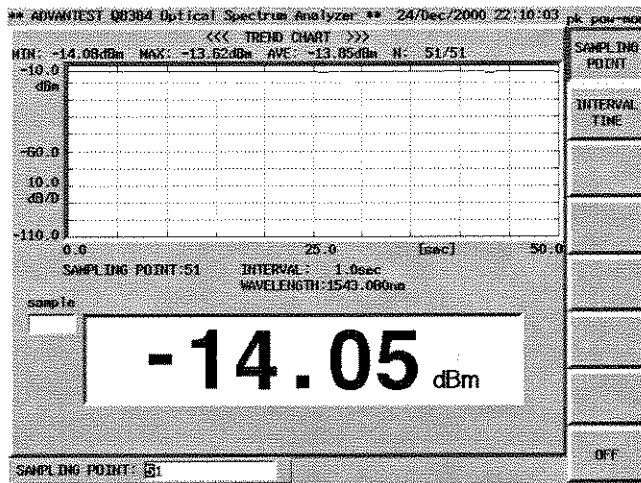


Figure 2-29 Displaying Input Light Changes in Time

---

**CAUTION:** *The peak power monitor function measures the spectrum internally and displays the peak level. The span, the resolution and the number of sampling points that were used immediately before the peak power monitor was started are used as the measurement conditions. As a result, to make the interval time shorter, set the values used immediately before the peak power monitor was started to smaller values.*

---



---

**CAUTION:** *When the span is set to 20 nm or more (when the number of sample points is 501) and peak powers are monitored, the measurement time may exceed the set time interval. If this occurs, an error message "INTERVAL TIME IS TOO SHORT" is displayed and measurements displayed do not match the time scale. Make the time interval longer.*

---

2.2.4 Alignment

### 2.2.4 Alignment

This function adjusts the optical axis of the monochromator used with the optical spectrum analyzer.

---

**CAUTION:** *Prior to operating this instrument immediately after having transported it with fierce vibrations, or operating this instrument in a place having abrupt temperature changes, be sure to warm up the instrument and then perform the AUTO ALIGNMENT function in advance.*

---

Power on

1. Turn the **POWER** switch (on the front panel) on.  
The startup screen is displayed after the self-test has been completed.

---


**NOTE:** *A minimum warm-up time of 30 minutes is required prior to making measurements.*

---

Setup

Use the light source from either the OUTPUT-2 connector (EE-LED output available as an option of this instrument) or an LD light source having a wavelength range of 1.2 to 1.65  $\mu\text{m}$ .

2. Connect the SM fiber cable from the light source to the optical input connector.

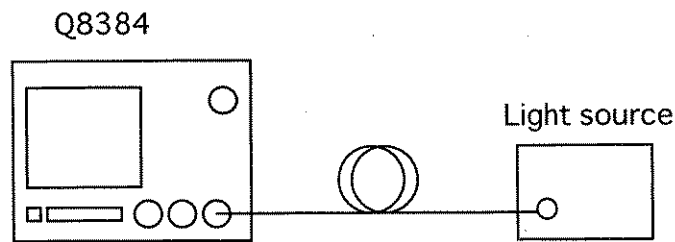

**Figure 2-30 Connecting the Calibration Signal**

3. Press **CAL** and **AUTO ALIGNMENT**.  
The optical axis alignment starts automatically, and is completed in approximately 30 seconds with a message indicating that the alignment has been completed is then displayed.

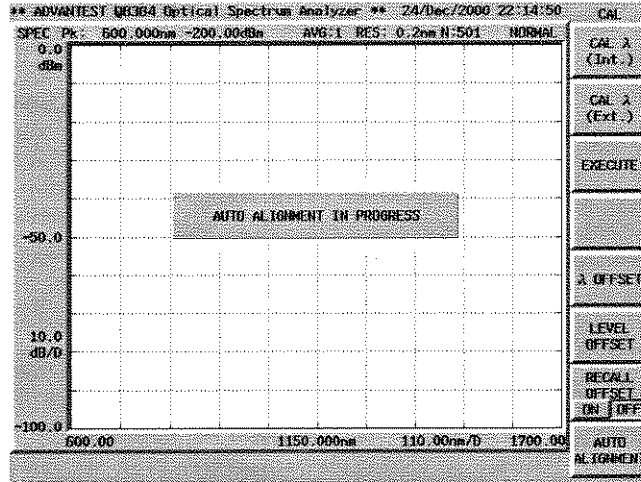


Figure 2-31 Alignment Execution Message

2.2.5 Calibration

2.2.5 Calibration

This section describes how to calibrate the instrument to keep the wavelength accuracy.

To make measurements accurately, use the optical spectrum analyzer at temperatures within the specified range.

Allow at least 30 minutes for the analyzer to warm up before performing a calibration.

There are two types of calibration for the optical spectrum analyzer.

- (a) Calibration using the built-in light source (Option)
- (b) Calibration using an external light source

(a) Calibration using the built-in light source (Option)

Power on

1. Turn the **POWER** switch (on the front panel) on.  
The startup screen is displayed after the self-test has been completed.

Initialization

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The initial settings are read.  
Allow at least 30 minutes for the analyzer to warm up before performing a calibration.

Setup

Connect the calibration signal to the optical spectrum analyzer.

3. Connect the optical fiber cable from the **OUTPUT-1** connector to the **INPUT** connector.

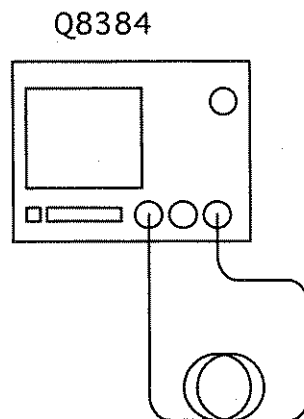


Figure 2-32 Connecting the Calibration Signal

## Executing the calibration operation

4. Press **CAL**, **CAL  $\lambda$  (Int.)** and **EXECUTE**.

A message is displayed and shows that calibration is in progress as shown below. About 90 seconds later, another message indicating that calibration is finished is displayed.

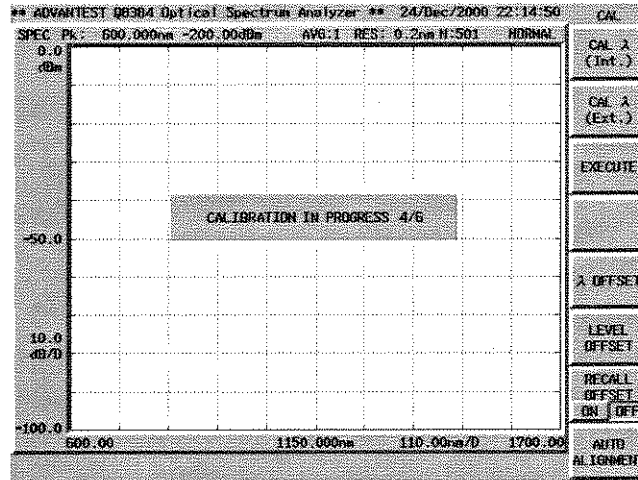


Figure 2-33 Calibration Execution Message

(b) Calibration using an external light source

## Power on

1. Turn the **POWER** switch (on the front panel) on.  
The startup screen is displayed after the self-test has been completed.

## Initialization

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The initial settings are read.  
Allow at least 30 minutes for the analyzer to warm up before performing a calibration.

## Connecting the calibration signal

3. Connect the single mode optical fiber cable from the external calibration light source to the optical spectrum analyzer **INPUT** connector.  
Use a laser caused by single wavelength oscillation as the light source.

2.2.5 Calibration

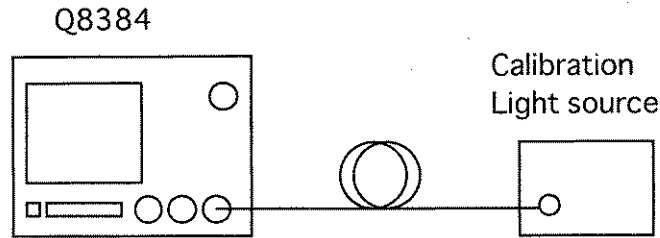


Figure 2-34 Connecting the Calibration Signal

4. Change the settings so that an external calibration light source spectrum can be displayed, and then measure the spectrum.

Executing the calibration operation

5. Press **CAL** and **CAL λ (Ext.)**.  
The input window is displayed.
6. Enter the wavelength of the calibration light source.

Perform a calibration so that the light source peak wavelength matches the wavelength entered from the input window.

7. Press **CAL** and **EXECUTE**.  
A message is displayed and shows that calibration is in progress as shown below. About 20 seconds later, another message indicating that calibration is finished is displayed.

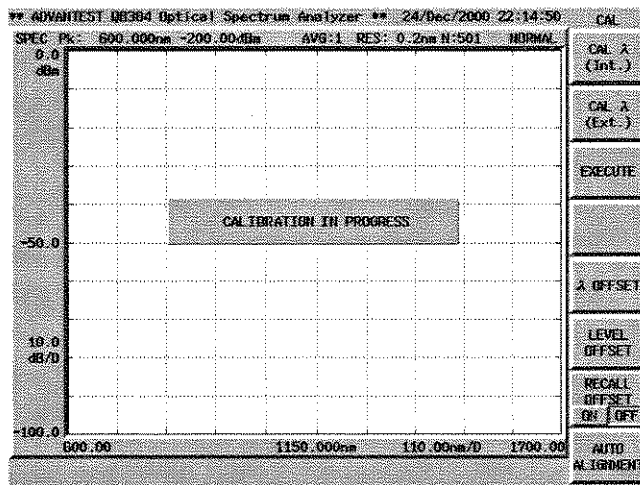


Figure 2-35 Calibration Execution Message

## 2.2.6 Measuring the Transmission-wavelength (or Loss-wavelength) Characteristics

**2.2.6 Measuring the Transmission-wavelength (or Loss-wavelength) Characteristics**

The NORMALIZE (LOSS/TRANS) function is used to display measurement data after it has been normalized with the data in reference memory or the spectrum maximum value.

This function is useful for measuring transmission-wavelength and loss-wavelength characteristics of parts such as optical fibers and optical filters after the output from OUTPUT-2 (on the optical spectrum analyzer) or a white light source has been connected to the input terminal (on the optical spectrum analyzer).

This section describes how to measure the transmission-wavelength (or loss-wavelength) characteristics of DUTs.

**Power on**

1. Turn the **POWER** switch (on the front panel) on.  
The startup screen is displayed after the self-test has been completed.


**Initialization**

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The initial settings are displayed.

**Saving the normalization data**

3. Connect the SM optical fiber from the light source **OUTPUT** connector to the optical spectrum analyzer **INPUT** connector.

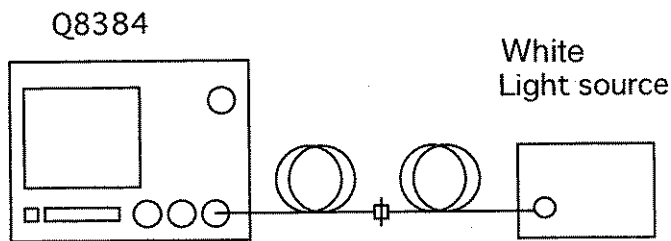

**Figure 2-36 Connecting the White Light Source**

This changes the analyzer settings so that the characteristics of a DUT may be displayed more clearly.

4. Press **CENTER**, **1**, **,**, **5**, **5** and **μm**.  
A center wavelength of 1.55 μm is set.
5. Press **SPAN**, **5**, **0**, and **nm**.  
An analysis span of 50 nm is set.
6. Press **SWEEP MODE** and **ADAPIVE**.  
The sweep mode is set to the adaptive mode.



2.2.6 Measuring the Transmission-wavelength (or Loss-wavelength) Characteristics

7. Press **SINGLE**.  
A sweep is performed.
8. Press **NORMALIZE LOSS/TRANS** and **SAVE REF DATA**.  
The spectrum data used as the reference data is saved to the memory.

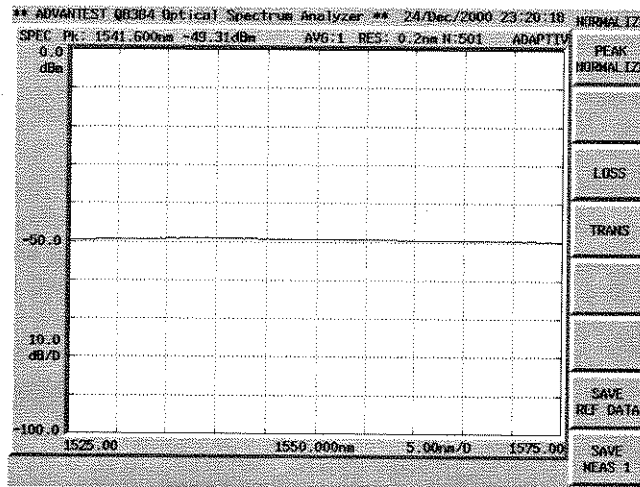


Figure 2-37 Saving the Reference Spectrum

Connecting a DUT

9. Replace the adapter currently connected with a DUT.

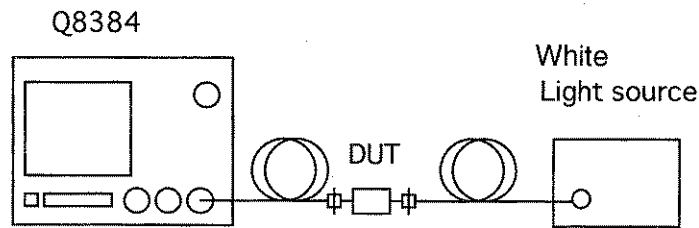


Figure 2-38 Connecting the White Light Source

Measuring the transmission-wavelength characteristics

10. Press **SINGLE**.  
A sweep is performed.
11. Press **NORMALIZE LOSS/TRANS** and **TRANS**.  
A waveform (current spectrum/Ref. Spectrum) showing transmission-wavelength characteristics is displayed.

2.2.6 Measuring the Transmission-wavelength (or Loss-wavelength) Characteristics

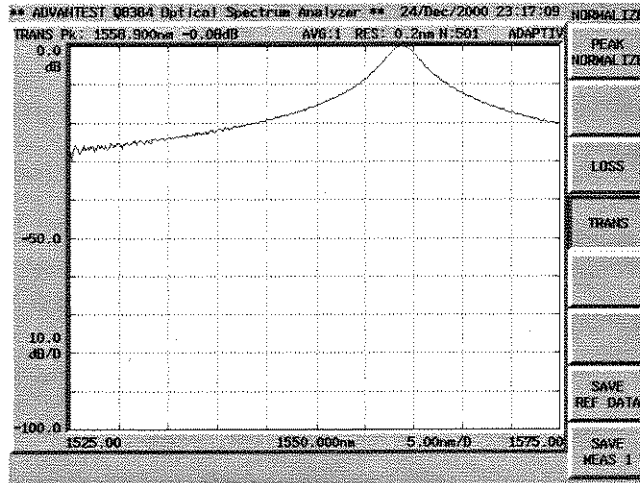


Figure 2-39 Transmission-wavelength Characteristics  
(Zooming function with LOSS/TRANS)

Measuring the loss-wavelength characteristics

12. Press **NORMALIZE LOSS/TRANS** and **LOSS**.  
A waveform (current spectrum or Ref. Spectrum) showing transmission-wavelength characteristics is displayed.

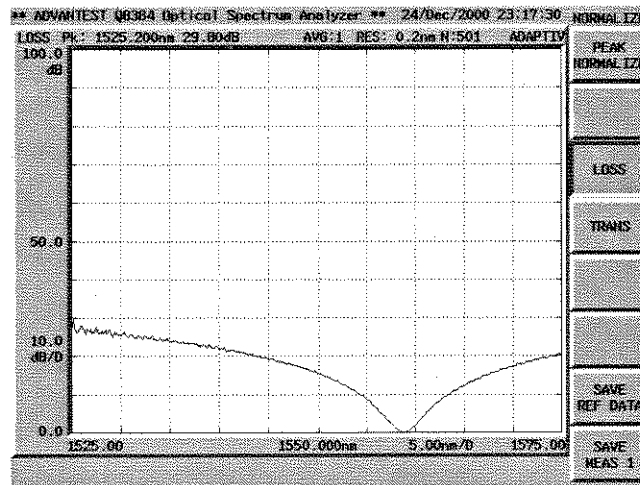


Figure 2-40 Loss-wavelength Characteristics  
(Zooming function with LOSS/TRANS)

Setting the REF LEVEL on the display

This changes the reference level on the screen so that the signals can be observed more easily.

13. Press **REF LEVEL, 4, 0** and **ENTER**.  
The reference level is set to 40 dB in the upper part of the screen.

## 2.2.6 Measuring the Transmission-wavelength (or Loss-wavelength) Characteristics

- The LOSS/TRANS function allows the same wavelengths to be used, each of which were measured from two different measurement condition groups for CENTER and SPAN, for an operation if the wavelength range set for reference memory is wider than the wavelength range of the current signal spectrum.  
As a result, we recommend that a wide wavelength range of a spectrum be specified in reference memory to avoid erasing the data in reference memory every time you change measurement conditions (refer to Section 5.5, "Auto-Panning and Auto-Zooming Functions")

## 2.2.7 Light Amplifier Characteristic Analysis

This section describes how to measure the gain and SNR of light amplifiers used for WDM (wavelength division multiplex) communications.

Measurement conditions: The target of the measurement is a light amplifier used for 1.55  $\mu\text{m}$  WDM (wavelength division multiplex) communications.  
Use appropriate parameter values when making the measurements in the example shown below.

### Power on

1. Turn the **POWER** switch (on the front panel) on.  
The startup screen is displayed after the self-test has been completed.

### Initialization

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The initial settings are read.

### Setting the measurement conditions

This changes the analyzer settings so that the input signal is displayed more clearly.

3. Press **CENTER, 1, ,, 5, 5** and  **$\mu\text{m}$** .  
A center wavelength of 1.55  $\mu\text{m}$  is set.
4. Press **SPAN, 8** and **nm**.  
An analysis span of 8 nm is set.
5. Press **REF LEVEL, 1, 0** and **dBm**.  
The reference level is set to 10 dBm.
6. Press **RESOLUTION** and **0, ,, 1** and **nm**.  
A resolution of 0.1 nm is set.

### Measuring the input signal to the light amplifier

7. Connect the optical fiber cable from the light source output connector to the optical spectrum analyzer **INPUT** connector.
8. Press **SINGLE**.  
A sweep is performed and the spectrum is displayed.

2.2.7 Light Amplifier Characteristic Analysis

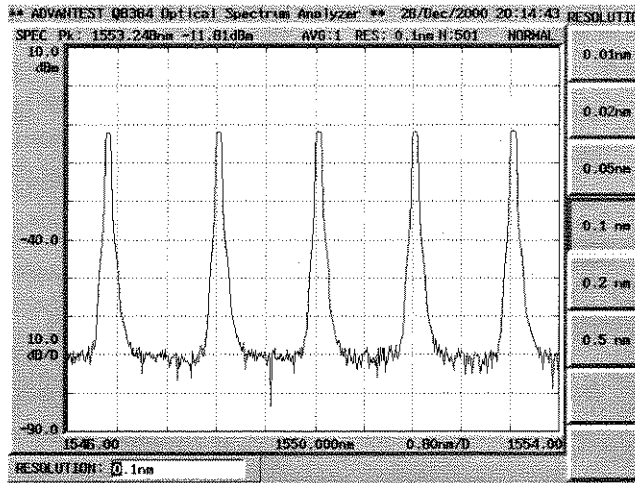


Figure 2-41 Measuring the Input Signal

Saving the reference data

9. Press **APPLICATION**, *opt.amp* and **MODE SNG/WDM** (WDM).  
Because this procedure uses different wavelength signals, WDM is selected.
10. Press **SAVE Pin**→**REF DATA**.  
The data associated with the input to the light amplifier is saved as reference data.

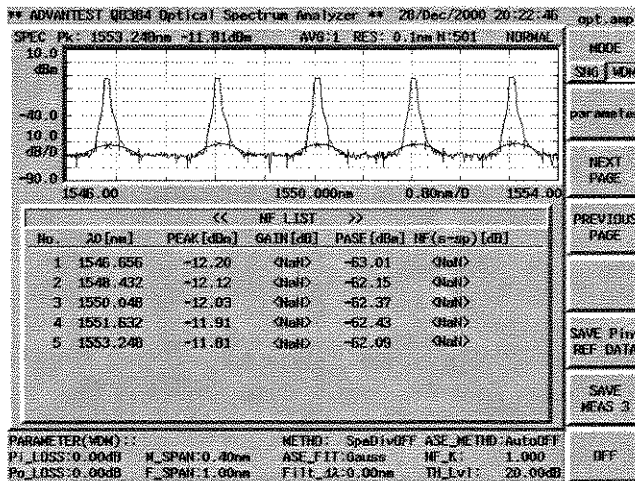


Figure 2-42 Saving the REF Data

Measuring the output signal of the light amplifier

11. Connect the optical fiber cable from the light source output connector to the light amplifier **INPUT** connector.
12. Connect the optical fiber cable from the light amplifier output connector to the optical spectrum analyzer **INPUT** connector.

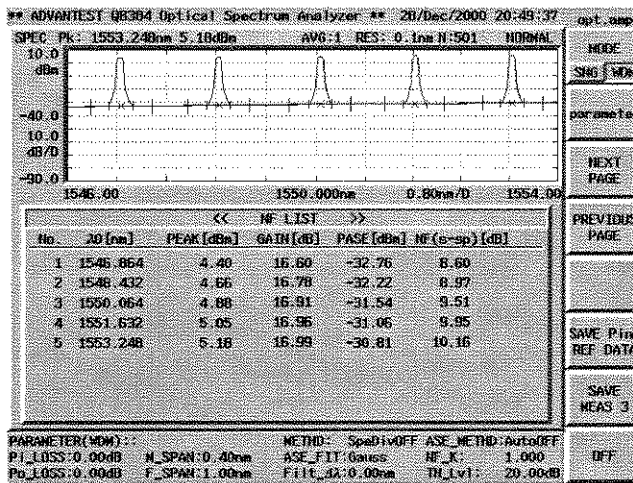


Figure 2-43 Measuring the Output Signal

13. Press **SINGLE**.  
A sweep is performed. The gain and NF are calculated and the resulting spectrum is displayed.

Setting the analysis conditions

14. Press **parameter**.  
The Optical AMP PARAMETER dialog box is displayed.

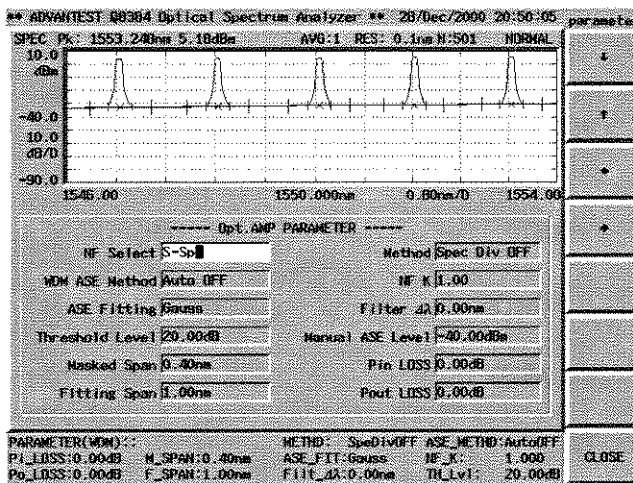


Figure 2-44 Optical AMP PARAMETER Dialog Box

To change parameters in the dialog box, move the cursor using the arrow key menu, select a parameter and specify a value using the arrows next to the text box, data knob or numeric keypad.

### 2.2.7 Light Amplifier Characteristic Analysis

15. Select **ASE FITTING** and set it to **Gauss**.  
The approximate expression used to calculate the ASE point becomes a Gaussian function.
16. Select **Masked Span** and set it to 1 nm.
17. Select **Fitting Span** and set it to 2 nm.
18. Select **Pin LOSS** (correction value for optical amplifier input loss in the measurement system), and set it to 0 dB.
19. Select **Pout LOSS** (correction value for optical amplifier output loss in the measurement system), and set it to 0 dB.
20. Select **FILTER  $\Delta\lambda$**  (optical receiver's light-intercepting band when NF SELECT is set to total), and set it to 0 dB.

For further information about step 15. to 20. above, refer to 5.4 GAIN&NF and SNR.

## 2.2.8 WDM Light Signal Characteristic Analysis

This section describes how to analyze main parameters of WDM light signals.

**Measurement conditions:** The target of the measurement is a WDM light signal source which has five channels and can generate light signals with a wavelength of  $1.55\ \mu\text{m}$  and an output level of  $+10\ \text{dBm}$ .

Use appropriate parameter values when making the measurements in the example shown below.

### Power on

1. Turn the **POWER** switch (on the front panel) on.  
The startup screen is displayed after the self-test has been completed.


### Initialization

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The initial settings are read.

### Connecting the input signal

3. Connect the optical fiber cable from the light source output connector to the optical spectrum analyzer **INPUT** connector.

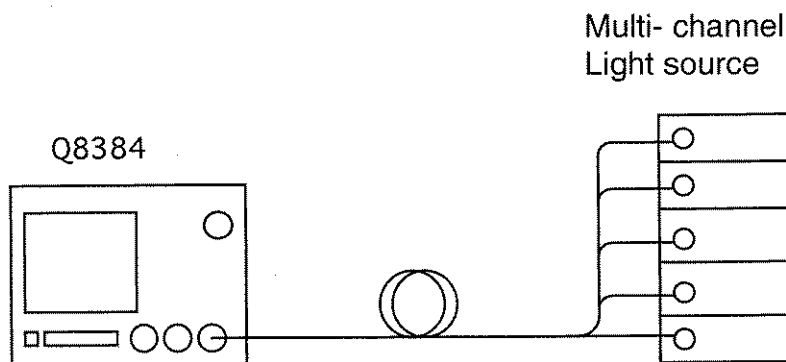

**Figure 2-45 Input Signal Connections**

### Setting the measurement conditions

This changes the analyzer settings so that the input signal is displayed more clearly.

4. Press **CENTER**, **1**, **.**, **5**, **5** and  **$\mu\text{m}$** .  
A center wavelength of  $1.55\ \mu\text{m}$  is set.



2.2.8 WDM Light Signal Characteristic Analysis

5. Press **SPAN, 5** and **nm**.  
An analysis span of 5 nm is set.  
Set up the optical spectrum analyzer so that all channels in a WDM signal to be analyzed are displayed.
6. Press **REF LEVEL, +, 2, 0** and **dBm**.  
The reference level is set to +20 dBm.
7. Press **RESOLUTION, 0, ., 0, 5** and **nm**.  
A resolution of 0.05nm is set.

Performing the measurement

8. Press **SINGLE**.  
A sweep is performed and the spectrum is displayed.

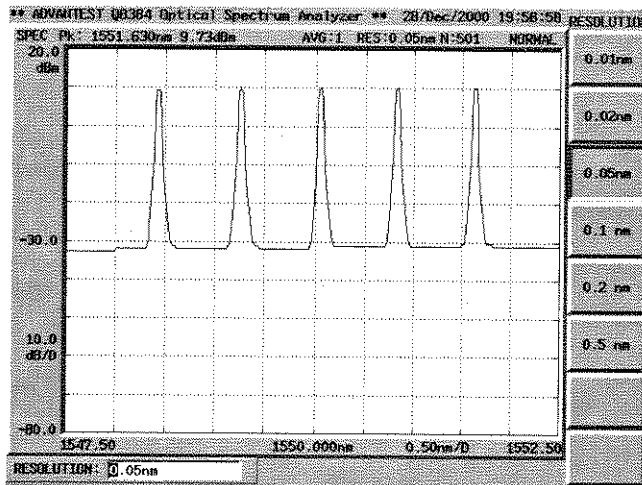


Figure 2-46 Measuring the Input Signal

Analyzing the wavelength and level of a WDM signal

9. Press **APPLICATION, wdm** and **MULTI PEAK**.  
Wavelengths and levels of peaks are displayed in a list at the bottom of the screen. Channel numbers are given starting from 1 in ascending order of wavelength or frequency.  
Up to eight sets of signal data can be displayed simultaneously. If there are more than eight sets of signal data, they can be displayed using **NEXT PAGE** or **PREVIOUS PAGE**.  
In addition, pressing **LIST ALL** displays a list over the entire screen that can contain up to 24 sets of signal data.

---

**CAUTION:** When the command **SAVE** is executed in **LIST ALL** mode, data is saved to a floppy disk as list data (extension: **.WDM**) in **ASCII** format so that it can be loaded into an external PC. Note that this data cannot be reloaded into this analyzer.

---

2.2.8 WDM Light Signal Characteristic Analysis

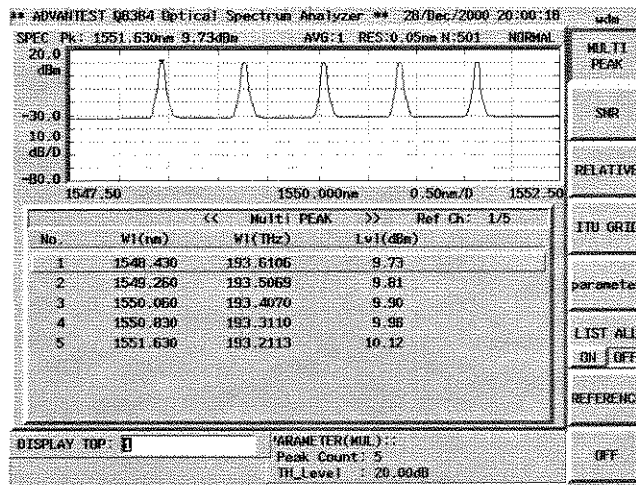


Figure 2-47 Displaying Multiple Peaks

Analyzing the difference in wavelength and the difference in level between two spectral peaks

10. Press **RELATIVE**.  
The wavelength and the level are displayed for each spectral peak. The difference in wavelength and the difference in level between the peak you selected and the reference peak are displayed. Signal No. 01 is set as the reference peak.
11. Press **REFERENCE**, then either step key ( $\Delta$  or  $\nabla$ ).  
The reference peak wavelength selection is changed accordingly.

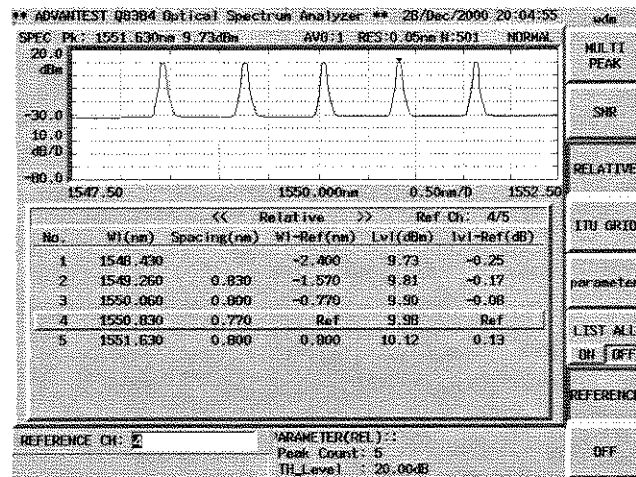


Figure 2-48 Displaying Relative Values

2.2.8 WDM Light Signal Characteristic Analysis

Analyzing the SNR

12. Press **SNR**.  
The Pass and SNR are displayed for each spectral peak.

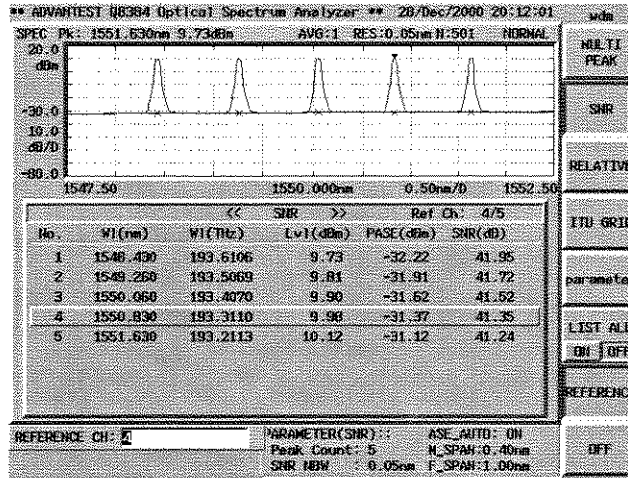


Figure 2-49 SNR

### 2.2.9 WDM Optical Signal Measurements Using the Monitoring Function

This section describes the monitoring function that is used to automatically measure a WDM signal the specified number of times at constant intervals.

Measurement conditions: The measurement signal used in this example is a WDM optical signal with: a wavelength of 1.55  $\mu\text{m}$  band, and 12 channels.

#### Power on

1. Turn the **power** switch (on the front panel) on.  
The startup screen is displayed when the self test is completed.

#### Initialization

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The initial settings are read.

#### Connecting the input signal

3. Connect the optical fiber cable from the light source output connector to the optical spectrum analyzer **INPUT** connector.

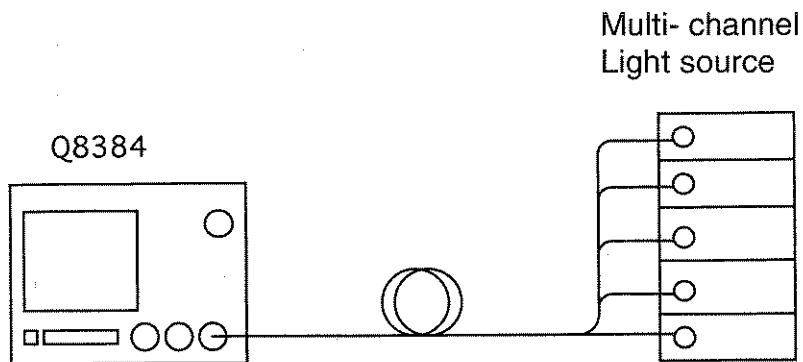


Figure 2-50 WDM Signal Connections

#### Setting the measurement conditions

This changes the analyzer settings so that the input signal is displayed more clearly.

4. Press **CENTER, 1, ,, 5, 5** and  **$\mu\text{m}$** .  
A center wavelength of 1.55  $\mu\text{m}$  is set.
5. Press **SPAN, 1, 0** and **nm**.  
An analysis span of 10 nm is set.

2.2.9 WDM Optical Signal Measurements Using the Monitoring Function

6. Press **REF LEVEL, 0** and **dBm**.  
The reference level is set to 0 dBm.
7. Press **RESOLUTION, 0, ,, 1** and **nm**.  
A resolution of 0.1 nm is set.

Performing the measurement

8. Press **SINGLE**.  
A sweep is performed and the spectrum is displayed.

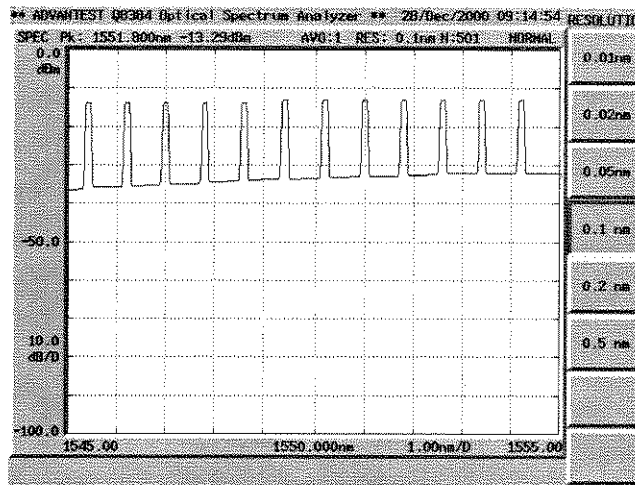


Figure 2-51 Measuring the Spectrum of a WDM Signal

Setting the measurement interval and the number of times the measurement is repeated

9. Press **APPLICATION** and *wdm monitor*.  
The WDM monitor screen is displayed.

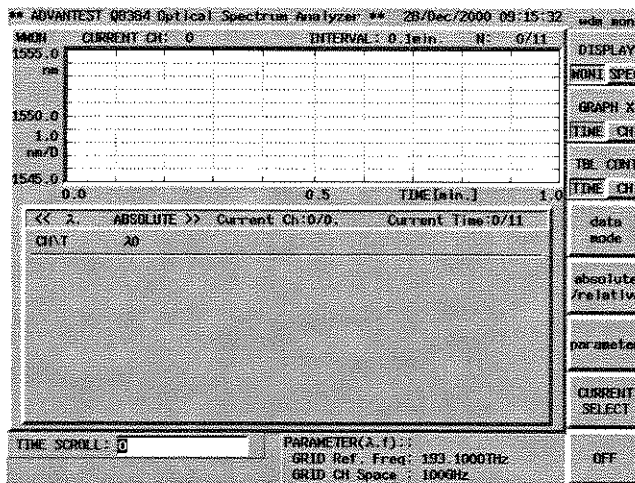


Figure 2-52 WDM Monitor Screen

## 2.2.9 WDM Optical Signal Measurements Using the Monitoring Function

10. Press **Parameter**.

The WDM monitor parameter dialog box is displayed.

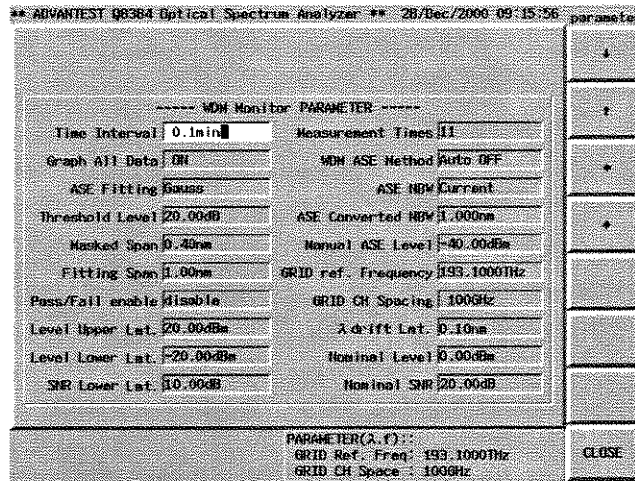


Figure 2-53 WDM Dialog Box Screen

11. Move the input cursor to Time Interval using the arrow keys on the soft keys.
12. Press **1** and **ENTER**.  
The measurement interval is set to 1 minute.
13. In the same manner, move the input cursor to Measurement Times.
14. Press **2, 1** and **ENTER**.  
The number of times is set to 21.
15. In the same manner, move the cursor to Graph All Data.
16. Turn Graph All Data off, using the step keys.  
The graph drawn only by the current data is displayed in the upper part of the screen.
17. In the same manner, move the cursor to Nominal Level.
18. Press **-, 1, 3** and **dBm**.  
Nominal level is set to -13 dBm.
19. Press **CLOSE**.  
This operation closes the parameter dialog box and displays the WDM monitor screen.

2.2.9 WDM Optical Signal Measurements Using the Monitoring Function

20. Press **SINGLE**.  
 (The **REPEAT** key is disabled when the instrument set to the WDM monitor function.)  
 The WDM monitor measurement is started and the measurement is taken the specified number of times.  
 The graph in the upper part of the screen indicates wavelength changes in the current channel optical signal along the time axis.  
 (The current channel is set to the first channel as the initial value.)  
 The wavelength measurement results for all channels are listed in absolute values in the table.

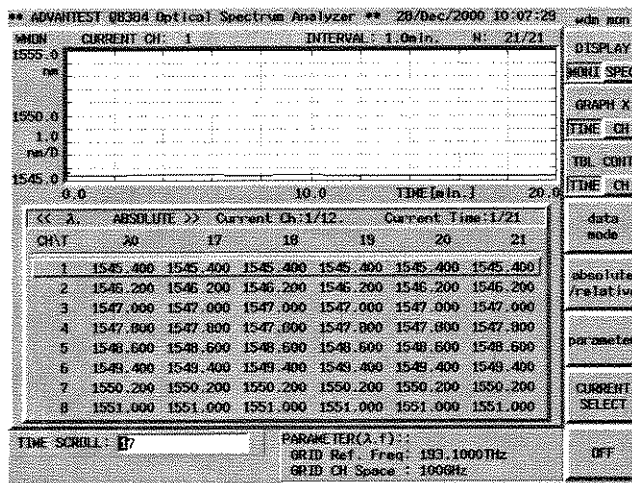


Figure 2-54 WDM Monitor Measurement Screen

21. The table data is scrolled to the top along the time axis using the arrow keys.  
 (Pressing **TBL CONT TIME/CH** toggles the scroll mode between channel and time.)

Data analysis

Measurement data can be displayed in various modes.

22. Press **data mode** and **SNR**.  
 The table data is now displayed as SNR for each channel, and the graph is displayed as the SNR changes for the current channel (along the time axis).  
 In this case, the vertical range of a graph is within Nominal SNR  $\pm$  10 dB.

2.2.9 WDM Optical Signal Measurements Using the Monitoring Function

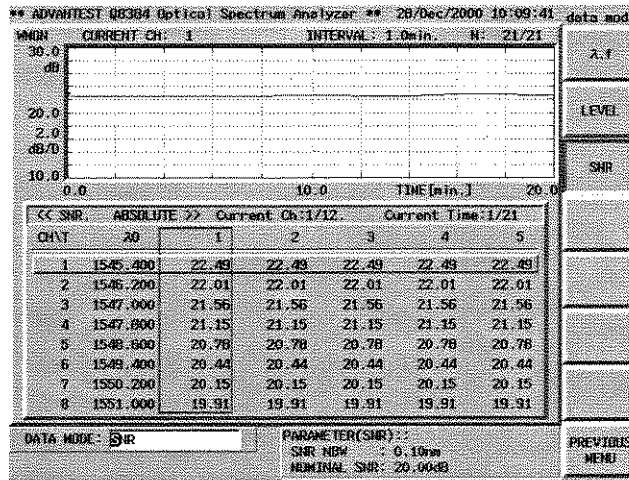


Figure 2-55 Displaying WDM Monitor SNR

23. Press **LEVEL**.

The table data is displayed as the signal level for each channel, and the graph is displayed as signal level changes for the current channel (along the time axis). In this case, the vertical range of a graph is within Nominal Level  $\pm 10$  dB.

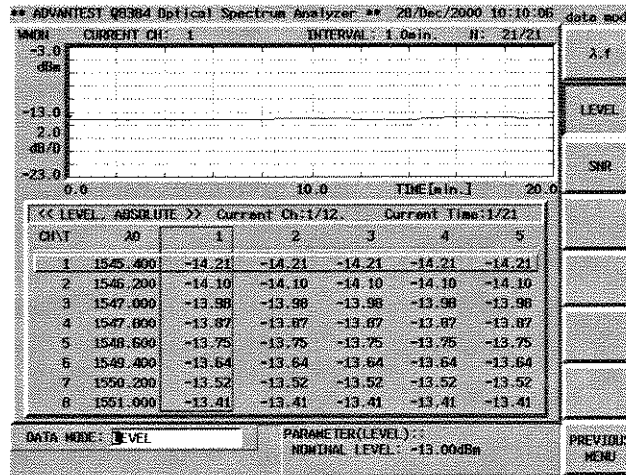


Figure 2-56 Displaying WDM Monitor Level

24. Press **PREVIOUS MENU**, *absolute/relative* and **INITIAL**.

The data is displayed as a value difference with respect to the first measurement value for each channel in a WDM signal. The graph is displayed in the same manner. In this case, the vertical range of a graph is within  $\pm 10$  dB.



2.2.9 WDM Optical Signal Measurements Using the Monitoring Function

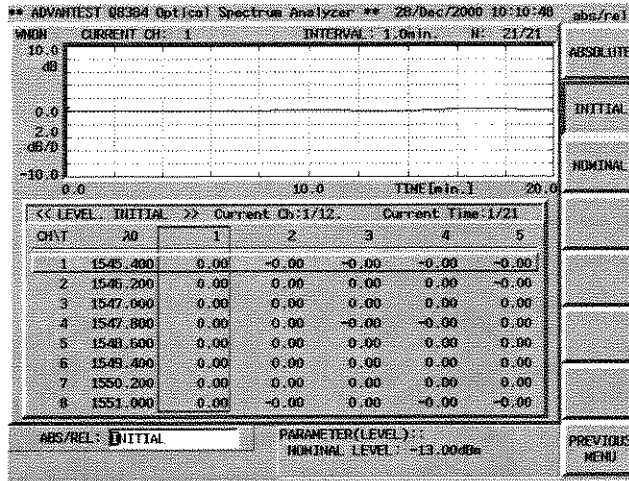


Figure 2-57 Displaying WDM Monitor Relative Values (INITIAL)

25. Press **NOMINAL**.

The data is displayed as the difference between Nominal LEVEL specified by parameter and the signal level for each channel. The graph is displayed in the same manner.

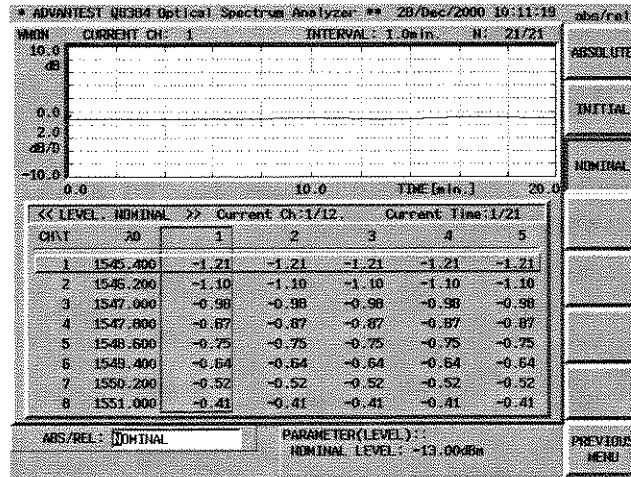


Figure 2-58 Displaying WDM Monitor Relative Values (NOMINAL)

26. Press **PREVIOUS MENU** and **GRAPH X TIME/CH**.

The horizontal axis represents the channel, and the data at the current time (the data for the first measurement is saved as the initial values) is displayed for each channel. The current channel is indicated with a marker.

## 2.2.9 WDM Optical Signal Measurements Using the Monitoring Function

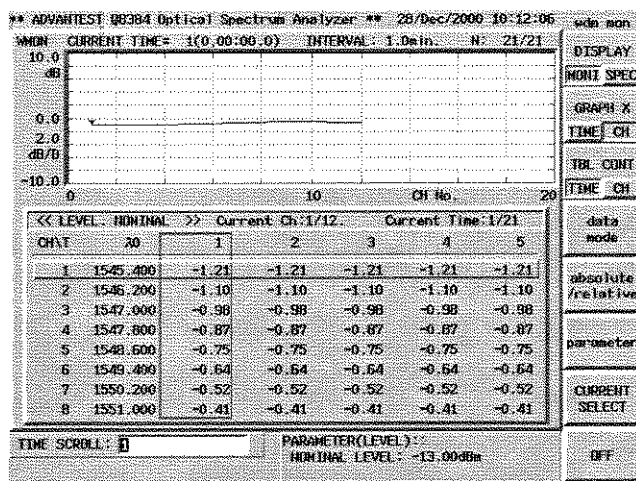


Figure 2-59 Displaying WDM Monitor Channels

27. Press **CURRENT SELECT**.

The data for an arbitrary time can be referred to by changing the current time with the arrow keys.

(Pressing **TBL CONT TIME/CH** toggles the current selection between channel and time.)

---

**CAUTION:** When the command **SAVE** is executed in the WDM monitor function, data is saved to a floppy disk as table data (extension: .WMN) in ASCII format so that it can be loaded into an external PC. Note that this data cannot be reloaded into this analyzer.

---

2.2.10 Limit Line Function for Device Evaluation

**2.2.10 Limit Line Function for Device Evaluation**

This section describes how to use the limit line function (used to make a Pass/Fail judgement based on the limit line).

Measurement conditions: Evaluating the transmission characteristics of a 1.55-nm-band bandpass filter.

Power on

1. Turn on the **POWER** switch (on the front panel).  
When the self-test has completed, the startup screen is displayed.


Initialization

This resets the current settings to the initial settings.

2. Press **INSTR PRESET** and **PRESET**.  
The INSTR PRESET menu is displayed.

Measuring the reference signal

3. Connect the SM fiber from the **OUTPUT** connector of the white light source to the **INPUT** connector on the optical spectrum analyzer.

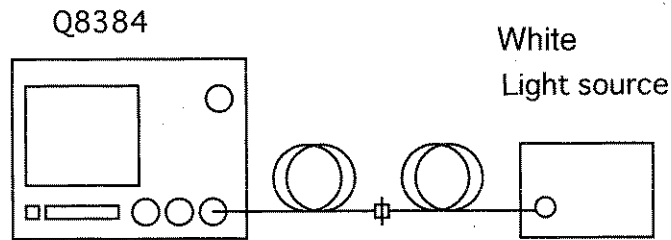

**Figure 2-60 Measuring the Reference Data Used for Filter Transmission Characteristics**

Measurement conditions are set so that the characteristics of a DUT can easily be observed.

4. Press **CENTER, 1, ., 5, 5** and **μm**.  
A center frequency of 1.55 μm is set.
5. Press **SPAN, 5, 0** and **nm**.  
An analysis span of 50 nm is set.
6. Press **REF LEVEL, -, 2, 0** and **dBm**.  
The reference level is set to -20 dBm.
7. Press **SWEEP MODE** and **ADAPTIVE**.
8. Press **RESOLUTION, 0, ., 5** and **nm**.  
A resolution of 0.5 nm is set.
9. Press **SINGLE**.

The measurement is made

10. Press **NORMALIZE LOSS/TRANS** and **SAVE REF DATA**.  
The reference spectrum data is saved in the memory.
11. Press **TRANS**.  
The measurement mode is changed to the transmission characteristic.  
(The reference waveform disappears and the transmission characteristic measurement mode is turned on.)

#### Setting the judgment criteria

Insert a floppy disk, which contains the judgment reference data file is saved, into the drive.

12. Press **ADVANCE**, *limit line* and **LOAD PATTERN FILES**.  
(For information on how to create the judgment reference data, refer to Section 5.7, "Setting Limit Line.")  
Load the judgment reference data from the floppy disk.

#### Selecting the judgment reference data

13. Press **PATTERNS**.  
The fifth file of the previously loaded criteria files (filename: "lmtln5.txt") is selected. The criteria in the previously selected file is displayed on the measurement screen.  
(If the criteria are not displayed, the settings for the criteria file and the settings for the optical spectrum analyzer do not match.)

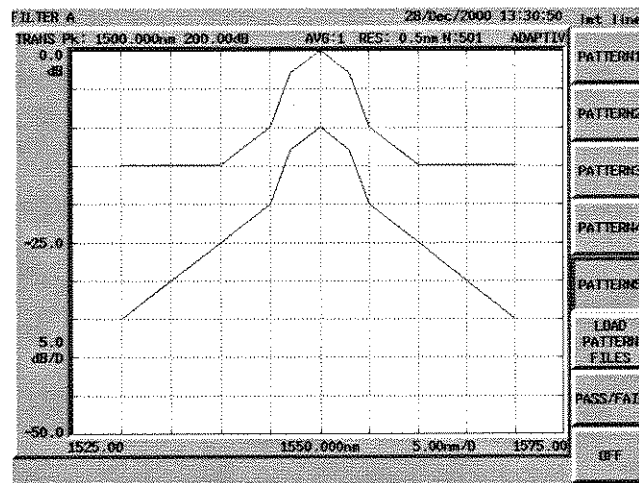


Figure 2-61 Displaying the Limit Line

2.2.10 Limit Line Function for Device Evaluation

Connecting the DUT

- 14. Connect the DUT.

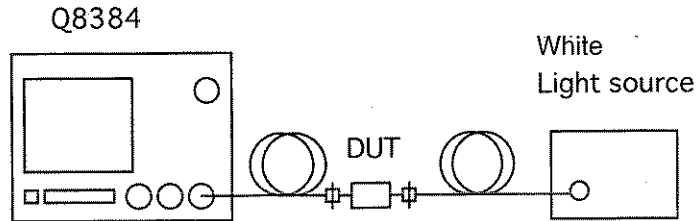


Figure 2-62 Connections Used for Device Evaluation

Transmission Characteristic Measurement

- 15. Press **SINGLE**.  
Start the measurement.

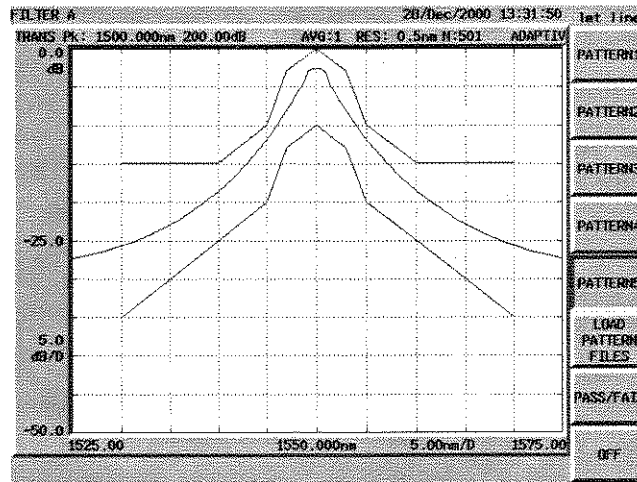


Figure 2-63 Transmission Characteristics of a Device to Be Evaluated (with the Limit Line Displayed)

- 16. Press **PASS/FAIL**.  
This operation makes a Pass/Fail judgement based on the judgment criteria.

## 2.2.11 Setting Measurement Conditions

This section describes the method of how to set measurement conditions for each item.

### (1) Changing the horizontal axis unit

The horizontal axis of the optical analyzer can be toggled between the wavelength and the frequency when the measurement mode is set to Spectrum, Transmission or Loss Mode.

Setting the horizontal axis to the wavelength

1. Press **SPAN**.
2. Set **WAVE/FREQ nm/THz** to **nm**.

Setting the horizontal axis to the frequency

1. Press **SPAN**.
2. Set **WAVE/FREQ nm/THz** to **THz**.

### (2) Setting the center wavelength or the center frequency

Setting the center wavelength using a numeric value and a unit

1. Press **CENTER**.
2. Enter a numeric value and a unit.  
(If the horizontal axis is set to the wavelength, it can be adjusted in increments of 0.001 nm. If the horizontal axis is set to the frequency, it can be rounded off in increments equivalent to 0.001 nm.)

To set the wavelength (or frequency) at the maximum peak to the center wavelength (or frequency)

1. Press **CENTER** and **PEAK→CENTER**.

To set the center wavelength (or frequency) to the wavelength (or frequency) specified by the cursor

1. Move the X cursor to the desired wavelength (or frequency).
2. Press **CENTER** and **CURSOR→CENTER**.  
When two X Cursors are displayed, the center wavelength or frequency is changed so that it is at the center of the wavelength or frequency between the two X Cursors.

## 2.2.11 Setting Measurement Conditions

### (3) Setting the analysis span

Setting the span using a numeric value and a unit

1. Press **SPAN**.
2. Enter a numeric value and a unit.  
(If the horizontal axis is set to the wavelength, it can be adjusted in increments of 0.1 nm. If the horizontal axis is set to the frequency, it can be rounded off in increments equivalent to 0.1 nm.)

Setting the span with a numeric value

1. Press **SPAN** and **START**.
2. Enter a numeric value and a unit.
3. Press **STOP**.
4. Enter a numeric value and a unit.

Setting the analysis span to the span specified by the X cursors

1. Determine the desired span using two X cursors.
2. Press **SPAN** and **CURSOR SPAN**.

### (4) Setting the reference level

Setting the span using a numeric value and a unit

1. Press **REF LEVEL**.
2. Enter a numeric value and a unit.

Setting the reference level to the level at the maximum peak

1. Press **REF LEVEL** and **PEAK→REF LEVEL**.

Setting the reference level to the level specified by the cursor

1. Move the Y cursor to the desired wavelength.
2. Press **REF LEVEL** and **CURSOR→REF LEVEL**.

## Setting a level range using two Y cursors

1. Determine the desired span using two Y cursors.
2. Press **REF LEVEL** and **CURSOR→REF LEVEL**.  
A view range is set as shown below depending on the types of level display.

## For LINEAR scale display

The reference level is set to the value indicated by the upper Y cursor, and the minimum level is set to the value indicated by the lower Y cursor.

## For LOG scale display

The reference level is set to the value indicated by the upper Y cursor, and **LEVEL SCALE** is optimized automatically according to the level difference between the two cursors.

---

**NOTE:** *The optical analyzer automatically controls the input sensitivity so that the output signal reaches a suitable level.  
(The REF LEVEL set during sweeps does not affect the measured trace.)*

---

## (5) Setting the vertical axis

The vertical axis of the optical analyzer can be toggled between LINEAR and LOG Scales.

## Setting the vertical axis to LINEAR Scale

1. Press **LEVEL SCALE**.
2. Set **LEVEL SCALE LIN/LOG** to LIN.

## Setting the vertical axis to LOG Scale

1. Press **LEVEL SCALE**.
2. Set **LEVEL SCALE LIN/LOG** to LOG.

When the vertical axis set to the LOG scale, set the scale as follows.

## Setting the scale using the soft key

1. Select a soft key from **10 dB/D**, **5 dB/D**, **2 dB/D**, **1 dB/D**, **0.5 dB/D**, **0.2 dB/D** and **0.1 dB/D**.

## Setting the scale by entering a value and its unit

1. Enter a value and its unit (in increments of 0.1 dB).



## 2.2.11 Setting Measurement Conditions

### (6) Setting the measurement resolution

Setting the resolution using the soft key

1. Press **RESOLUTION**.
2. Select an appropriate key from 0.01 nm, 0.02 nm, 0.05 nm, 0.1 nm, 0.2 nm and 0.5 nm.

Setting a value

1. Press **RESOLUTION**.
2. Enter a value and its unit (Any values are rounded down to 1, 2 or 5.).

### (7) Setting the measurement points

Selecting the point using the soft key

1. Press **CONTROL** and *sampling point*.
2. Select an appropriate key from 101, 201, 501, 1001, 2001, 5001 and 10001.

Setting a value

1. Press **CONTROL** and *sampling point*.
2. Enter a value and press the **ENTER**.  
(the value you entered is automatically replaced by one of the values that is the closest to the value you entered: 101, 201, 501, 1001, 2001, 5001 or 10001).

### (8) Setting the averaging count

There are two types of averaging functions: the point averaging and sweep averaging functions. The point averaging function sets the sampling integration time (of the power measurement) proportional to the number of averaging. The sweep averaging function calculates the average power for each sampling point after sweeping the specified number of times. Choose a function as desired to improve the accuracy of low or unstable power level measurement.

Setting the number of point averaging

How to make settings using the soft keys

1. Press **AVG**, *point average*.
2. Select a soft key from *1, 2, 4, 8, 16, 32* and *64*.

How to make settings by entering a value

1. Press **AVG** and *point average*.
2. Enter a value and press the **ENTER** (this function is turned off if you enter 1).

Setting the number of sweep averaging

How to make settings using the soft key

1. Press **AVG** and *sweep average*.
2. Select a soft key from *1, 2, 4, 8, 16, 32* and *64*.

How to make settings by entering a value

1. Press **AVG** and *sweep average*.
2. Enter a value and press the **ENTER** (this function is turned off if you enter 1).

(9) Setting the number of smoothing points

The optical spectrum analyzer has a function to obtain smoothed spectrums using the moving average.

Set the computing range for moving average (up to 11 points) if necessary, although smoothing is not normally required.

Setting the smoothing function

How to make settings using the soft key

1. Press **AVG** and *smoothing*.
2. Select a soft key from *1, 3, 5, 7, 9* and *11*.

How to make settings by entering a value

1. Press **AVG** and *smoothing*.
2. Enter a value and press the **ENTER** (A value entered is rounded up to an odd number between 3 and 11. If 1 is entered, this function is turned off).

(10) Setting the measurement mode

Choose the measurement mode according to the characteristics of the light under measurement and the sweep time.

For the measurement modes, refer to Section 5.1, "Measurement Modes."

2.2.11 Setting Measurement Conditions

(11) Sweeping

For a single sweep

1. Press **SINGLE**.

For repeated sweeps

1. Press **REPEAT**.

Stopping sweeping

1. Press **STOP**.

## 2.3 Using Expanded Functions and Inputting/Outputting Data

### 2.3.1 Entering Label Data

This function is used to enter labels (messages of up to 48 characters) which serve as comments for measured data and are displayed at the top of the screen. The initial (or current) settings are as follows. When  $\alpha$ ,  $\beta$ ,  $\gamma$ ,  $\delta$ ,  $\lambda$ ,  $\mu$ ,  $\Delta$ ,  $\Lambda$ ,  $\Sigma$  and  $\int$  included in the character list (referred to as the character menu) are sent through GPIB, they changed to blank characters.

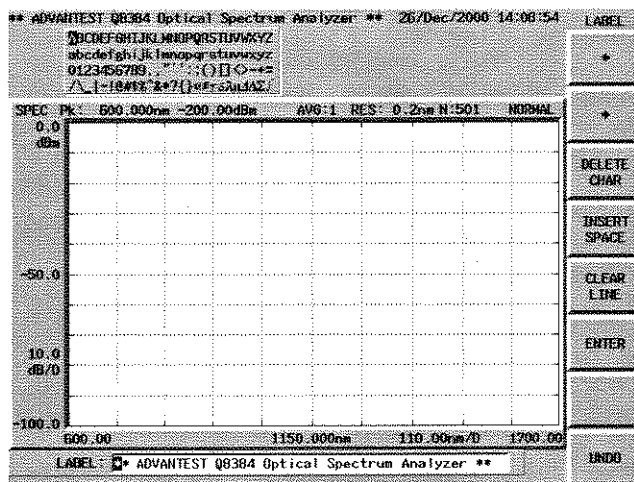


Figure 2-64 Label Data

#### Changing label data

The example shown below shows how to change the character string ADVANTEST to STAR by using the panel keys.

1. Press **LABEL**.  
A list of characters which can be entered (referred to as the character menu) is displayed at the top of the screen.  
The current label is displayed in the lower left-hand corner of the screen.
2. Position the cursor to the left of A of the character string ADVANTEST.
3. Select S from the character menu and press **ENTER**.
4. Repeat Step 3. until you finish to enter TAR.
5. Press **DELETE CHAR** five times to delete NTEST.
6. Press **ENTER** on the DATA section of the front panel to update the label.

After **LABEL** has been pressed, steps 2 thru 5 (or 6) can be performed directly from an external keyboard.

## 2.3.2 Selecting Color Patterns on the Screen

### 2.3.2 Selecting Color Patterns on the Screen

There are five color patterns and you can select any one from these patterns as follows: press **DEVICE**, *color* and select a pattern by pressing *PATTERN-1* through *PATTERN-5* as desired.

### 2.3.3 Setting Date/Time

The optical analyzer includes the clock function backed up by a battery.

#### Displaying Date and Time

1. Press **DEVICE**, *clock* and **DISPLAY ON/OFF(ON)**.  
Date and time are displayed in the upper right corner of the screen.  
As an example, set a time of 15:35 for September 20, 1999.

---

**NOTE:** To delete the displayed data, press **DISPLAY ON/OFF** again.

---

#### Altering the Date

2. Select **YEAR**, and set it to 1999, using the step keys or data knob.
3. Select **MONTH**, and set it to 9 September, using the step keys or data knob.
4. Select **DAY**, and set it to 20, using the step keys or data knob.

#### Altering the Time

5. Select **HOUR**, and set it to 15, using the step keys or data knob.
6. Select **MINUTE**, and set it to 35, using the step keys or data knob.

---

**NOTE:** Seconds are automatically set to 0 when the hour is changed.

---

## 2.3.4 Saving or Reading Data

### 2.3.4.1 Floppy Disk

The optical analyzer is equipped with a 3.5-inch floppy disk drive.

Measurement data, WDM list data and BMP data (screen display) can be saved to a floppy disk. Data saved to floppy disks can also be accessed from a personal computer.

3.5-inch DD 720 K or HD 1.44 MB (compliant with the MS-DOS format) can be used with the optical spectrum analyzer.

#### (1) Inserting Floppy Disks

1. Insert a floppy disk into the floppy disk drive with the label surface up.

#### (2) Removing Floppy Disks

1. Verify that the lamp on the drive is not lit and then remove the disk.

---

**CAUTION:** *Do not remove the floppy disk while the drive lamp is lit, since this indicates that floppy disk is being accessed. If you remove the disk while the disk is being accessed, you may damage the data contained on the disk.*

---

2. Press the eject button.  
The floppy disk is ejected from the drive.
3. Remove the disk from the drive.

#### (3) Formatting a Floppy Disk

To save data to a new floppy disk, be sure to format the floppy disk first. Use the following procedure to format a floppy disk.

---

**NOTE:** *Only DD 720 K or HD 1.44 MB floppy disks can be formatted. HD 1.2 MB floppy disks cannot be formatted.*

---

1. Make sure the write protection switch is unlocked.

---

**CAUTION:** *Formatting a floppy disk will erase any information stored on that disk, including the label Q8384.*

---

2. Insert the floppy disk into the disk drive.
3. Press **DEVICE**, *floppy* and *format*.
4. Press **EXECUTE** after selecting *2DD(720K)* or *2HD(1.44 M)*.

## 2.3.4 Saving or Reading Data

### 2.3.4.2 Backup Memory

The following data is stored in the backup memory: 15 or more screens (assuming a sampling of 501 sampling points) of measurement data.

### 2.3.4.3 Saving Data

Measurement data can be saved to the backup memory or to a floppy disk. This section describes the procedure used to save measurement data to the backup memory.

Selecting a device to save data

1. Press **SAVE** and **SAVE MEM/FDD(MEM)**.  
Backup memory is selected as the destination to save data.

Setting a file name

2. Press **SAVE**, *save meas data* and *name*.  
The character menu is displayed.  
For information on how to enter data, refer to Section 2.3.1, "Entering Label Data."
3. After typing the file name, press **ENTER** on the DATA section of the front panel.  
The file name is registered.
4. Execute **SAVE**.  
The file name is saved into the backup memory.

A file name can also be entered from an external keyboard.

The data saved on a floppy disk using the optical spectrum analyzer can be loaded into an external personal computer. Refer to Appendix A.4.

---

**NOTE:** *If you save data without specifying the file name, the center frequency of the file is saved as the file name.  
When the value which is going to be saved already exists, the last center frequency value added by 1 becomes the file name having a value between 001 and 999.*

---

### 2.3.4.4 Reading Data

This reads data from a floppy disk.

Selecting the device to be used

1. Press **RECALL** and **RECALL MEM/FDD(FDD)**.  
The floppy disk drive is selected as the device.

Selecting Data

2. Press **RECALL**, *recall meas data* and **RECALL**.  
The measurement data selected is recalled.  
The floppy disk file list is displayed on the screen.
3. Position the cursor on the name of the file you wish to open.
4. Press **RECALL**.  
The specified file is opened and the contents are displayed on the screen.



2.3.5 Outputting Data (Hard Copy)

2.3.5 Outputting Data (Hard Copy)

2.3.5.1 Internal printer

1. Press **DEVICE**, *select output* and **INTERNAL PRINTER**.  
The internal printer is selected as the output destination.
2. Press **DEVICE**, *printer* and **MENU OUT ON/OFF**.  
**MENU OUT ON/OFF** is used to set whether to output the soft menu.
3. Press **COPY**.  
The data is output to the internal printer.

2.3.5.2 External printer

This section describes how to print out screen data.

This analyzer system can output screen data to the provided printer using a parallel interface (compliant with the Centronics). Even though a color printer is connected to the analyzer, the printer prints out in monochrome.

---

**NOTE:** *The output resolution of this analyzer system is 180 dots/inch. Using a printer with a resolution other than integral multiples of 180 dots/inch may cause striped patterns to appear.*

---

Printers provided with ESC/P, ESC/P raster, or HP PCL as the printer control code can be used with this analyzer (some printer operations may be restricted).

Table 2-1 shows typical examples.

**Table 2-2 Recommended Printers**

Manufacturer	Model
EPSON	PM-750C (ESC/P R)
HEWLETT-PACKARD	DeskJet 694C, DeskJet 880L (PCL)
CANON	BJC-430J (ESC/P)

Connecting the printer

1. Connect the printer cable to the **PRINTER** connector on the rear panel.  
The printer cable specified by the printer manufacturer must conform to IBM-PC specifications.

---

**CAUTION:** *To prevent the units from being damaged, the printer cable should be connected after turning the power off.*

---

2. Press **DEVICE**, *select output* and **EXTERNAL PRINTER**.  
The external printer is selected as the output destination.

## Setting the Print Mode

3. Press **DEVICE**, *printer* and *external printer*.  
The soft menu used to select the print mode and the printer control code is selected.
4. Select **MODE:GRAY**, **MODE:MONO S** or **MODE:MONO L**.  
The grayscale, small monochrome or large monochrome output mode is selected.
5. Press one of **COMMAND:ESC/P**, **COMMAND:HP PCL** and **COMMAND:ESC/P RAS**.  
ESC/P, HP PCL or ESC/P RAS is enabled. The optical analyzer can use any of these printer control codes: ESC/P (Epson Standard Code for Printer), HP PCL (Hewlett Packard Printer Command Language) or ESC/P (Epson Standard Code for Printer Raster mode). Select the desired mode.
6. Press **DEVICE**, *printer* and **MENU OUT ON/OFF**.  
This turns MENU OUT on or off.

## Printing Data

7. Display the screen you wish to print and press **COPY**.  
The data is output to the external printer.

### 2.3.5.3 Floppy disk

The analyzer is used to save screen data in BMP (bitmap) format onto floppy disks so that the data can be loaded on an external computer. (The analyzer cannot be used to load data in BMP format.)

## Inserting a floppy disk

1. Insert a floppy disk into the floppy disk drive.

## Setting the destination device

2. Press **DEVICE**, *select output* and **FLOPPY DISK**.  
The floppy disk is selected as the output destination.

2.3.5 Outputting Data (Hard Copy)

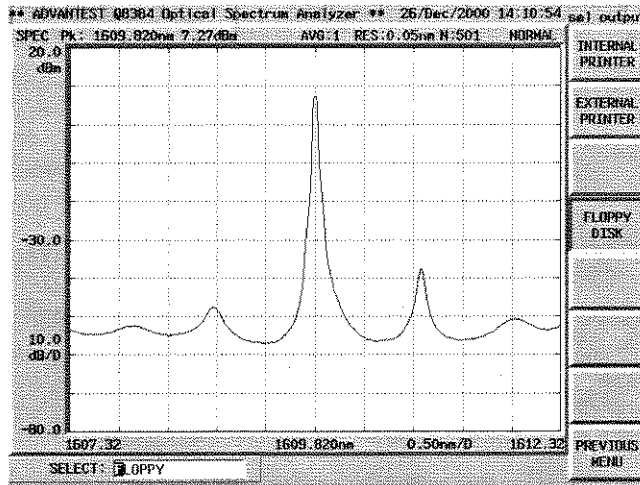


Figure 2-65 Selecting the Floppy Disk

3. Press **DEVICE**, *floppy*, *bit map* and **MODE:MONO**.  
The bitmap is saved in monochrome.
4. Press **DEVICE**, *floppy*, *bit map* and **COMPRESS ON/OFF**.  
This sets whether to compress the bit map.
5. Press **COPY** after displaying the screen data to be saved. The access lamp remains lit while the screen data is being saved to disk, and goes out when the file has been saved.

---

**CAUTION:** Do not remove the floppy disk while the access lamp is lit, since the floppy disk is being accessed. If you remove the disk while the disk is being accessed, you may damage the data on the disk.

---

### 3 REFERENCE

This chapter describes the functions of all panel and soft keys.

- Menu index: Use this index as a key index to Chapter 3.
- Menu map: Shows a list of hierarchical menus on a panel key basis.
- Functional descriptions: Explains the functions of the panel and soft keys.

#### 3.1 Menu Index

This menu index is used to easily find the keys described in Chapter 3.

Operation Key	Pages	Operation Key	Pages
$\Delta$ MODE .....	3-10, 3-34	10dB/D .....	3-5, 3-18
$\lambda$ drift Lmt. ....	3-9, 3-32	11 .....	3-6, 3-23
$\lambda$ OFFSET .....	3-14, 3-43	16 .....	3-6, 3-22
$\lambda.f$ .....	3-9, 3-29	1dB/D .....	3-5, 3-18
$\lambda 1$ .....	3-10	2 .....	3-6, 3-22
$\lambda 2$ .....	3-10	2001 .....	3-11, 3-36
← .....	3-8, 3-9, 3-12, 3-14, 3-26, 3-28, 3-30, 3-37, 3-44	201 .....	3-11, 3-36
↑ .....	3-8, 3-9, 3-26, 3-28, 3-30	2dB/D .....	3-5, 3-18
→ .....	3-8, 3-9, 3-12, 3-14, 3-26, 3-28, 3-30, 3-37, 3-44	2DD(720K) .....	3-13, 3-40
↓ .....	3-8, 3-9, 3-26, 3-28, 3-30	2HD(1.44M) .....	3-13, 3-40
0.01nm .....	3-6, 3-19	2ND PEAK .....	3-10, 3-34
0.02nm .....	3-6, 3-19	3 .....	3-6, 3-22
0.05nm .....	3-6, 3-19	32 .....	3-6, 3-22
0.1dB/D .....	3-5, 3-18	4 .....	3-6, 3-22
0.1nm .....	3-6, 3-19	5 .....	3-6, 3-22
0.2dB/D .....	3-5, 3-18	5001 .....	3-11, 3-36
0.2nm .....	3-6, 3-19	501 .....	3-11, 3-36
0.5dB/D .....	3-5, 3-18	5dB/D .....	3-5, 3-18
0.5nm .....	3-6, 3-19	64 .....	3-6, 3-22
1(OFF) .....	3-6, 3-22	7 .....	3-6, 3-23
10001 .....	3-11, 3-36	8 .....	3-6, 3-22
1001 .....	3-11, 3-36	9 .....	3-6, 3-23
101 .....	3-11, 3-36	ABORT .....	3-7, 3-23
		ABSOLUTE .....	3-9, 3-30
		absolute/relative .....	3-9, 3-30
		ACT U&L ON/OFF .....	3-11, 3-35
		ADAPTIVE .....	3-6, 3-20
		ADDRESS DOWN .....	3-14, 3-42
		ADDRESS UP .....	3-14, 3-42
		ADVANCE .....	3-10
		APPLICATION .....	3-8
		ASE Converted NBW .....	3-8, 3-9, 3-29, 3-32
		ASE Fitting .....	3-8, 3-9, 3-27, 3-28,

3.1 Menu Index

ASE NBW .....	3-8, 3-9, 3-29, 3-31	EXT KEY US/JP .....	3-13, 3-40
AUTO .....	3-7	EXTERNAL PRINTER .....	3-13, 3-39
AUTO ALIGNMENT .....	3-14, 3-43	external printer .....	3-13, 3-39
AUTO ON/OFF .....	3-11, 3-36	FEED .....	3-14
AUTO PKC ON/OFF .....	3-5, 3-15	Filter $\Delta\lambda$ .....	3-8, 3-27
AUTO RELV ON/OFF .....	3-5, 3-17	Fitting Span .....	3-8, 3-9, 3-27, 3-28
AUTO TRAC ON/OFF .....	3-11, 3-35	Fitting span .....	3-31
AVG .....	3-6	floppy .....	3-13, 3-39
BEEP ON/OFF .....	3-13, 3-41	FLOPPY DISK .....	3-13, 3-39
bit map .....	3-13, 3-40	format .....	3-13, 3-39
buzzer .....	3-13, 3-41	FULL SPAN .....	3-5, 3-16
CAL .....	3-14	GATE TIME .....	3-6, 3-21
CAL $\lambda$ (Ext.) .....	3-14, 3-43	Graph All Data .....	3-9, 3-30
CAL $\lambda$ (Int.) .....	3-14, 3-43	GRAPH X TIME/CH .....	3-9, 3-29
CENTER .....	3-5	GRID CH Spacing .....	3-8, 3-9, 3-29, 3-32
CLEAR LINE .....	3-14, 3-44	GRID ON/OFF .....	3-11, 3-35
clock .....	3-13, 3-40	GRID ref. Frequency .....	3-8, 3-9, 3-29, 3-32
CLOSE .....	3-8, 3-9, 3-26, 3-28	HEADER ON/OFF .....	3-14, 3-42
color .....	3-13, 3-40	HI DYNAMIC1 .....	3-6, 3-20
COMMAND:ESC/P .....	3-13, 3-39	HI DYNAMIC2 .....	3-6, 3-20
COMMAND:ESC/P RAS .....	3-13, 3-39	HI-SENS1 .....	3-6, 3-20
COMMAND:HP PCL .....	3-13, 3-39	HI-SENS2 .....	3-6, 3-20
COMPRESS ON/OFF .....	3-13, 3-40	HOUR .....	3-13, 3-41
CONTROL .....	3-11	INITIAL .....	3-9, 3-30
COPY .....	3-14	INSERT SPACE .....	3-14, 3-44
CURRENT SELECT .....	3-9, 3-32	INSTR PRESET .....	3-14
CURSOR SPAN .....	3-5, 3-16	INTERNAL PRINTER .....	3-13, 3-39
CURSOR→CENTER .....	3-5, 3-15	INTERVAL TIME .....	3-10, 3-33
CURSOR→REF LEVEL .....	3-5, 3-17	ITU GRID .....	3-8, 3-28
data mode .....	3-9, 3-29	K .....	3-8, 3-25
DAY .....	3-13, 3-41	Kr(RMS) .....	3-8, 3-25
DELAY .....	3-6, 3-20	L1 .....	3-10
DELETE .....	3-12, 3-37	L2 .....	3-10
DELETE ALL .....	3-11, 3-35	LABEL .....	3-14
DELETE CHAR .....	3-14, 3-44	LEFT PEAK .....	3-10, 3-34
DELETE CURRENT .....	3-11, 3-35	LEVEL .....	3-8, 3-9, 3-26, 3-30
DEVICE .....	3-13	Level Lower Lmt. ....	3-9, 3-31
DIRECTORY .....	3-13, 3-39	LEVEL OFFSET .....	3-14, 3-43
DISPLAY MONI/SPEC .....	3-9, 3-29	LEVEL SCALE .....	3-5
DISPLAY ON/OFF .....	3-13, 3-40	Level Upper Lmt. ....	3-9, 3-31
DUAL ON/OFF .....	3-11, 3-35	limit line .....	3-10, 3-33
EDGE RISE/FALL .....	3-6, 3-21	LIST ALL ON/OFF .....	3-8, 3-29
ENTER .....	3-12, 3-14, 3-37, 3-44	LOAD PATTERN FILES .....	3-10, 3-33
ENVELOPE .....	3-8, 3-25	LOCAL .....	3-14
EXECUTE .....	3-13, 3-14, 3-39, 3-43	LOSS .....	3-7, 3-24
EXIT .....	3-12, 3-37,	LVL SCALE LIN/LOG .....	3-5, 3-18

Manual ASE Level .....	3-8, 3-9, 3-27, 3-29, 3-32	Pass/Fail enable .....	3-9, 3-31
Masked Span .....	3-8, 3-9, 3-27, 3-28, 3-31	PATTERN-1 .....	3-13, 3-40
MAX HOLD ON/OFF .....	3-5, 3-17	PATTERN1 .....	3-10, 3-33
MAX HOLD→CURRENT .....	3-5, 3-17	PATTERN-2 .....	3-13, 3-40
Measurement Times .....	3-9, 3-31	PATTERN2 .....	3-10, 3-33
MENU OUT ON/OFF .....	3-13, 3-39	PATTERN-3 .....	3-13, 3-40
Method .....	3-8, 3-27	PATTERN3 .....	3-10, 3-33
MIN .....	3-17	PATTERN-4 .....	3-13, 3-40
MIN HOLD ON/OFF .....	3-5, 3-17	PATTERN4 .....	3-10, 3-33
MIN HOLD→CURRENT .....	3-5, 3-17	PATTERN-5 .....	3-13, 3-40
MINUTE .....	3-13, 3-41	PATTERN5 .....	3-10, 3-33
MODE SNG/WDM .....	3-8, 3-26	PEAK NORMALIZE .....	3-7, 3-24
MODE:COLOR .....	3-13, 3-40	peak power-mon .....	3-10, 3-33
MODE:GRAY .....	3-13, 3-39, 3-40	PEAK RMS .....	3-8, 3-25
MODE:MONO .....	3-13, 3-40	PEAK TO PEAK .....	3-10, 3-34
MODE:MONO L .....	3-13, 3-39	PEAK-THRESHOLD .....	3-8, 3-25
MODE:MONO S .....	3-13, 3-39	PEAK→CENTER .....	3-5, 3-15
MONTH .....	3-13, 3-40	PEAK→REF LEVEL .....	3-5, 3-17
MULTI PEAK .....	3-8, 3-28	Pin LOSS .....	3-8, 3-27
multi trace .....	3-11, 3-35	point average .....	3-6, 3-22
name .....	3-12, 3-37	Pout LOSS .....	3-8, 3-27
NAME CLEAR .....	3-12, 3-37	POWER .....	3-10, 3-34
NEXT .....	3-11, 3-35	PRESET .....	3-14, 3-42
NEXT PAGE .....	3-27	PREV .....	3-11, 3-35
NF K .....	3-8, 3-27	PREVIOUS PAGE .....	3-8, 3-27
NF Select .....	3-8, 3-26	printer .....	3-13, 3-39
NOMINAL .....	3-9, 3-30	PULSE .....	3-6, 3-20
Nominal Level .....	3-9, 3-32	QUIET ON/OFF .....	3-13, 3-41
Nominal SNR .....	3-9, 3-32	RECALL .....	3-12, 3-38
NORMAL .....	3-6, 3-10, 3-20, 3-34	RECALL MEAS 1 .....	3-12, 3-38
NORMALIZE LOSS/TRANS .....	3-7	RECALL MEAS 2 .....	3-12, 3-38
notch width .....	3-8, 3-26	RECALL MEAS 3 .....	3-12, 3-38
OFF .....	3-8, 3-9, 3-10, 3-11, 3-25, 3-26, 3-28, 3-29, 3-32, 3-33, 3-35	recall meas data .....	3-12, 3-38
ON/OFF .....	3-10	RECALL MEM/FDD .....	3-12, 3-38
opt.amp .....	3-8, 3-26	RECALL OFFSET ON/OFF .....	3-14, 3-43
parameter .....	3-6, 3-8, 3-9, 3-20, 3-25, 3-26, 3-28, 3-30	RECALL REF DATA .....	3-12, 3-38
PASS/FAIL .....	3-10, 3-33	RECOVER .....	3-12, 3-37
		REF LEVEL .....	3-5
		REFERENCE .....	3-8, 3-29
		RELATIVE .....	3-8, 3-28
		REPEAT .....	3-7
		RESOLUTION .....	3-6
		RIGHT PEAK .....	3-10, 3-34
		RMS .....	3-8, 3-25
		S.IMPOSE ON/OFF .....	3-11, 3-35
		SAMPLING POINT .....	3-10, 3-33
		sampling point .....	3-11, 3-35
		SAVE .....	3-12, 3-37
		SAVE MEAS 1 .....	3-7, 3-12, 3-24, 3-37
		SAVE MEAS 2 .....	3-12, 3-37



3.1 Menu Index

SAVE MEAS 3 .....	3-8, 3-12, 3-37
save meas data .....	3-12, 3-37
SAVE MEM 3 .....	3-27
SAVE MEM/FDD .....	3-12, 3-37
SAVE Pin→REF DATA .....	3-8, 3-27
SAVE REF DATA .....	3-7, 3-12, 3-24, 3-37
select output .....	3-13, 3-39
SELF TEST .....	3-14, 3-42
SINGLE .....	3-7
smoothing .....	3-6, 3-22
SNR .....	3-8, 3-9, 3-28, 3-30
SNR Lower Lmt. ....	3-9, 3-31
SPAN .....	3-5, 3-16
spectral width .....	3-8, 3-25
START .....	3-5, 3-7, 3-16, 3-23
STOP .....	3-5, 3-7, 3-16
sweep average .....	3-6, 3-22
SWEEP MODE .....	3-6
SYNC HI/LOW .....	3-6, 3-20
TBL CONT TIME/CH .....	3-9, 3-29
Threshold Level .....	3-8, 3-9, 3-27, 3-28, 3-31
THRESHOLD LVL1(dB) .....	3-8, 3-25
THRESHOLD LVL2(dB) .....	3-8, 3-25
Time Interval .....	3-9, 3-30
TRACE MAX .....	3-11, 3-35
TRANS .....	3-7, 3-24
UNDO .....	3-14, 3-44
WARNING ON/OFF .....	3-13, 3-41
WAVE/FREQ nm/THz .....	3-5, 3-16
wdm .....	3-8, 3-28
WDM ASE Method .....	3-8, 3-9, 3-27, 3-28, 3-31
wdm monitor .....	3-8, 3-29
WIDTH .....	3-8, 3-25, 3-26
X-CHANGE UPR/LOW .....	3-11, 3-35
XdB WIDTH .....	3-8, 3-26
Xnm LEVEL .....	3-8, 3-25, 3-26
YEAR .....	3-13, 3-40

## 3.2 Menu Map

This section shows the hierarchical menu configuration on a panel key basis.

---

**NOTE:**  Represents a panel key.  
 Represents a dialog box.  
 Unless otherwise noted, the soft menus are shown.

---

### CENTER




PEAK → CENTER  
 CURSOR → CENTER  
 AUTO PKC ON/OFF

### SPAN



SPAN  
 START  
 STOP  
 CURSOR SPAN  
 FULL SPAN  
 WAVE/FREQ nm/THz

### REF LEVEL



PEAK → REF LEVEL  
 CURSOR → REF LEVEL  
 MAX HOLD → CURRENT  
 MIN HOLD → CURRENT  
 MAX HOLD ON/OFF  
 MIN HOLD ON/OFF  
 AUTO RELV ON/OFF

### LEVEL SCALE




LVL SCALE LIN/LOG  
 10dB/D  
 5dB/D  
 2dB/D  
 1dB/D  
 0.5dB/D  
 0.2dB/D  
 0.1dB/D




3.2 Menu Map


**RESOLUTION**




**SWEEP MODE**

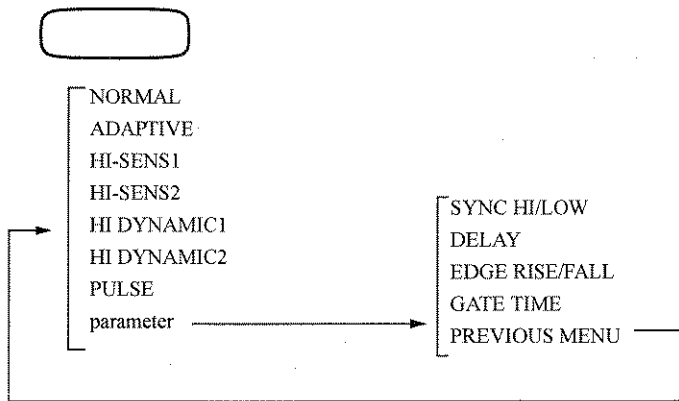

**AVG**

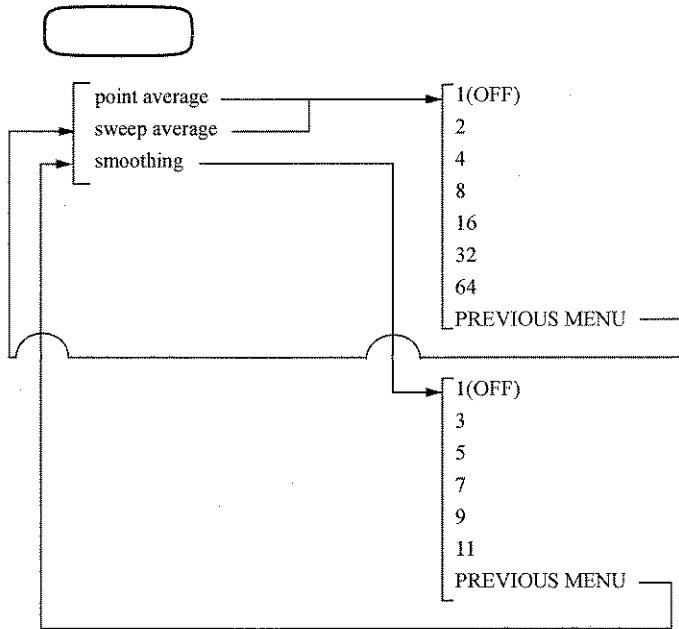

**AUTO**



START  
ABORT

**SINGLE**



**REPEAT**



**STOP**



**NORMALIZE  
LOSS/TRANS**



PEAK NORMALIZE  
LOSS  
TRANS  
SAVE REF DATA  
SAVE MEAS 1

3.2 Menu Map

APPLICATION



- spectral width
- notch width
- opt.amp
- wdm
- wdm monitor

- PEAK-THRESHOLD
- ENVELOPE
- RMS
- PEAK RMS
- Xnm LEVEL
- parameter
- OFF

- THRESHOLD LVL1(dB)
- THRESHOLD LVL2(dB)
- K
- Kr(RMS)
- WIDTH
- PREVIOUS MENU

- XdB WIDTH
- Xnm LEVEL
- parameter
- OFF

- LEVEL
- WIDTH
- PREVIOUS MENU

- MODE SNG/WDM
- parameter
- NEXT PAGE
- PREVIOUS PAGE
- SAVE Pin→REF DATA
- SAVE MEAS 3
- OFF

- ↓
- ↑
- ←
- 
- CLOSE


- NF Select
- WDM ASE Method
- ASE Fitting
- Threshold Level
- Masked Span
- Fitting Span
- Method
- NF K
- Filter  $\Delta\lambda$
- Manual ASE Level
- Pin LOSS
- Pout LOSS

- MULTI PEAK
- SNR
- RELATIVE
- ITU GRID
- parameter
- LIST ALL ON/OFF
- REFERENCE
- OFF


- ↓
- ↑
- ←
- 
- CLOSE

- WDM ASE Method
- ASE Fitting
- Threshold Level
- Masked Span
- Fitting Span
- ASE NBW
- ASE Converted NBW
- Manual ASE Level
- GRID ref. Frequency
- GRID CH Spacing


Next page

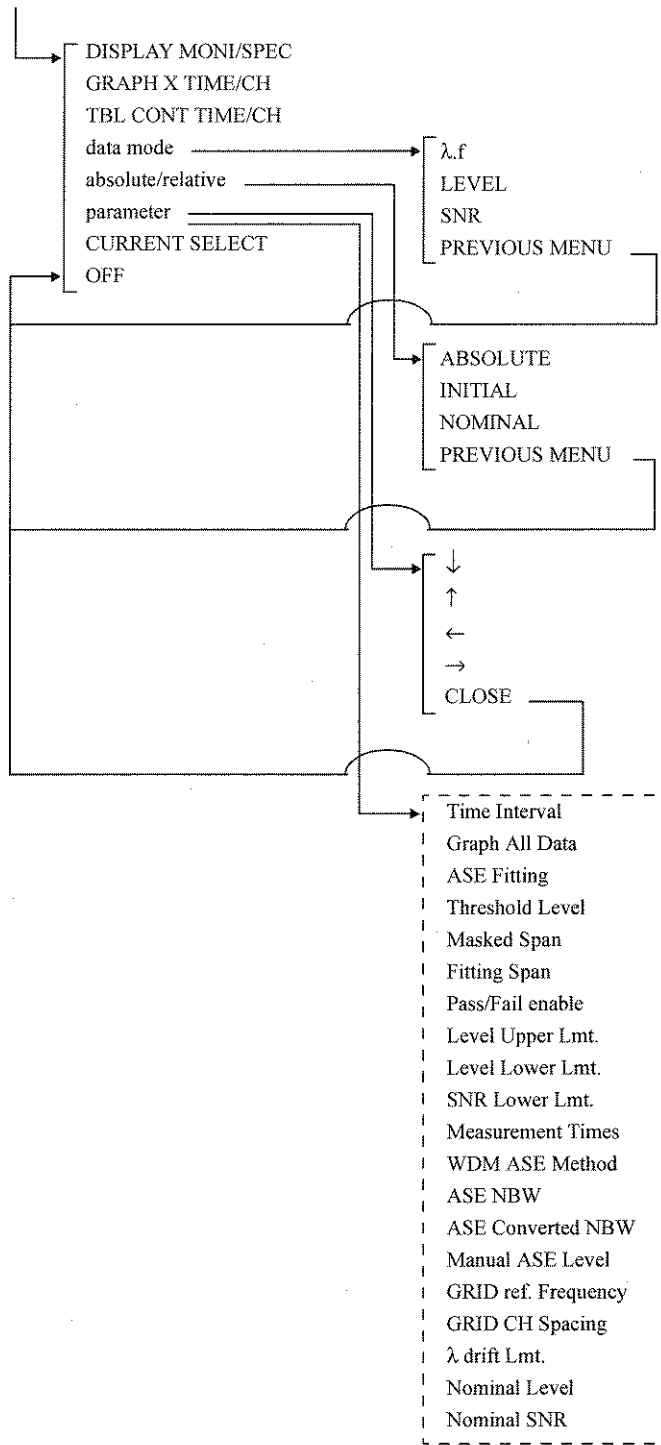

3.2 Menu Map

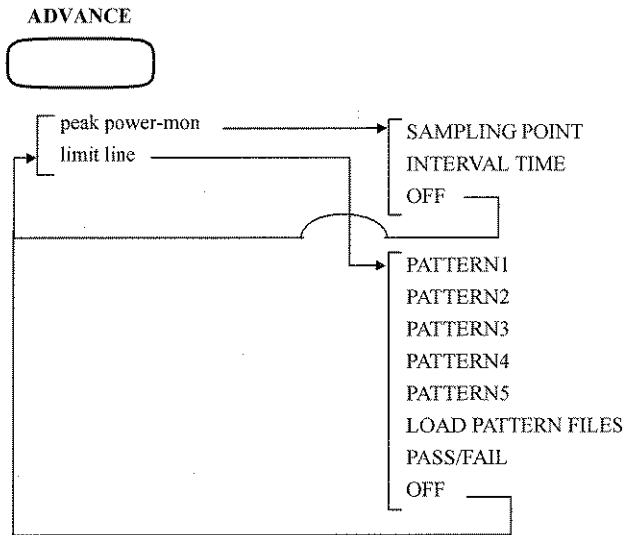


**ON/OFF** (CURSOR Section)

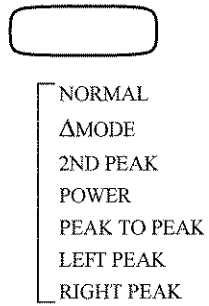

$\lambda 1$



$\lambda 2$




L1






L2



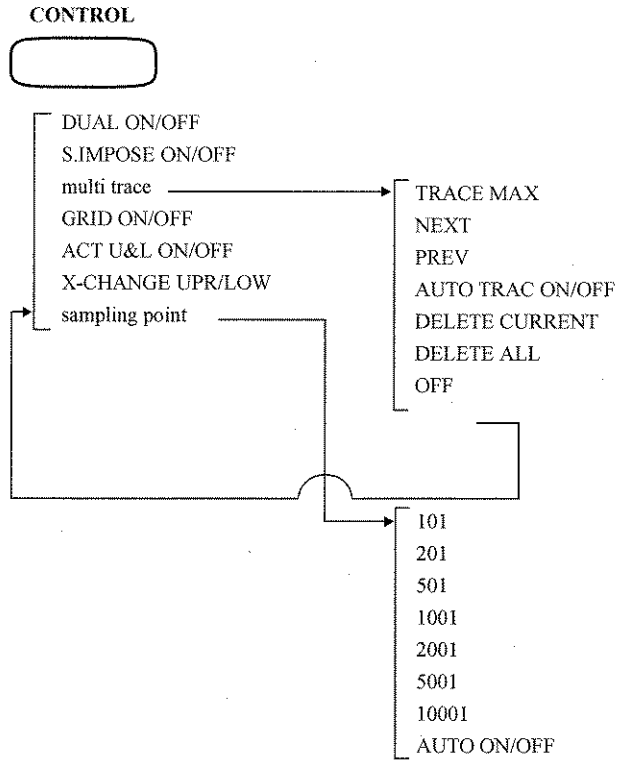

3.2 Menu Map

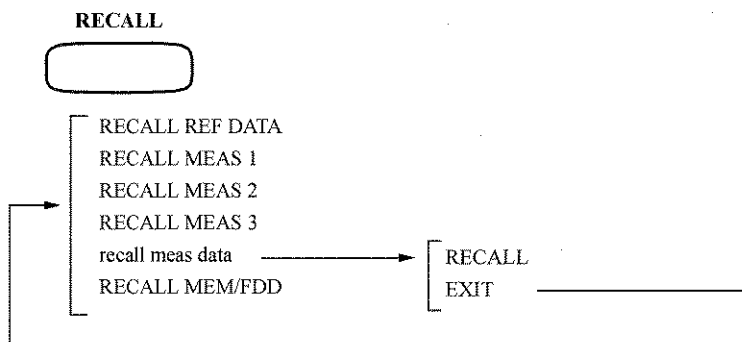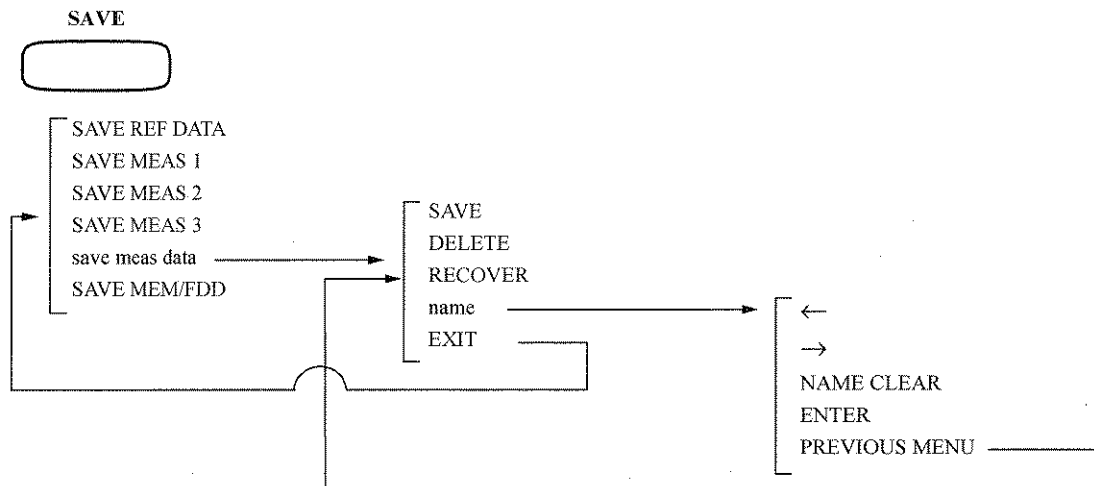

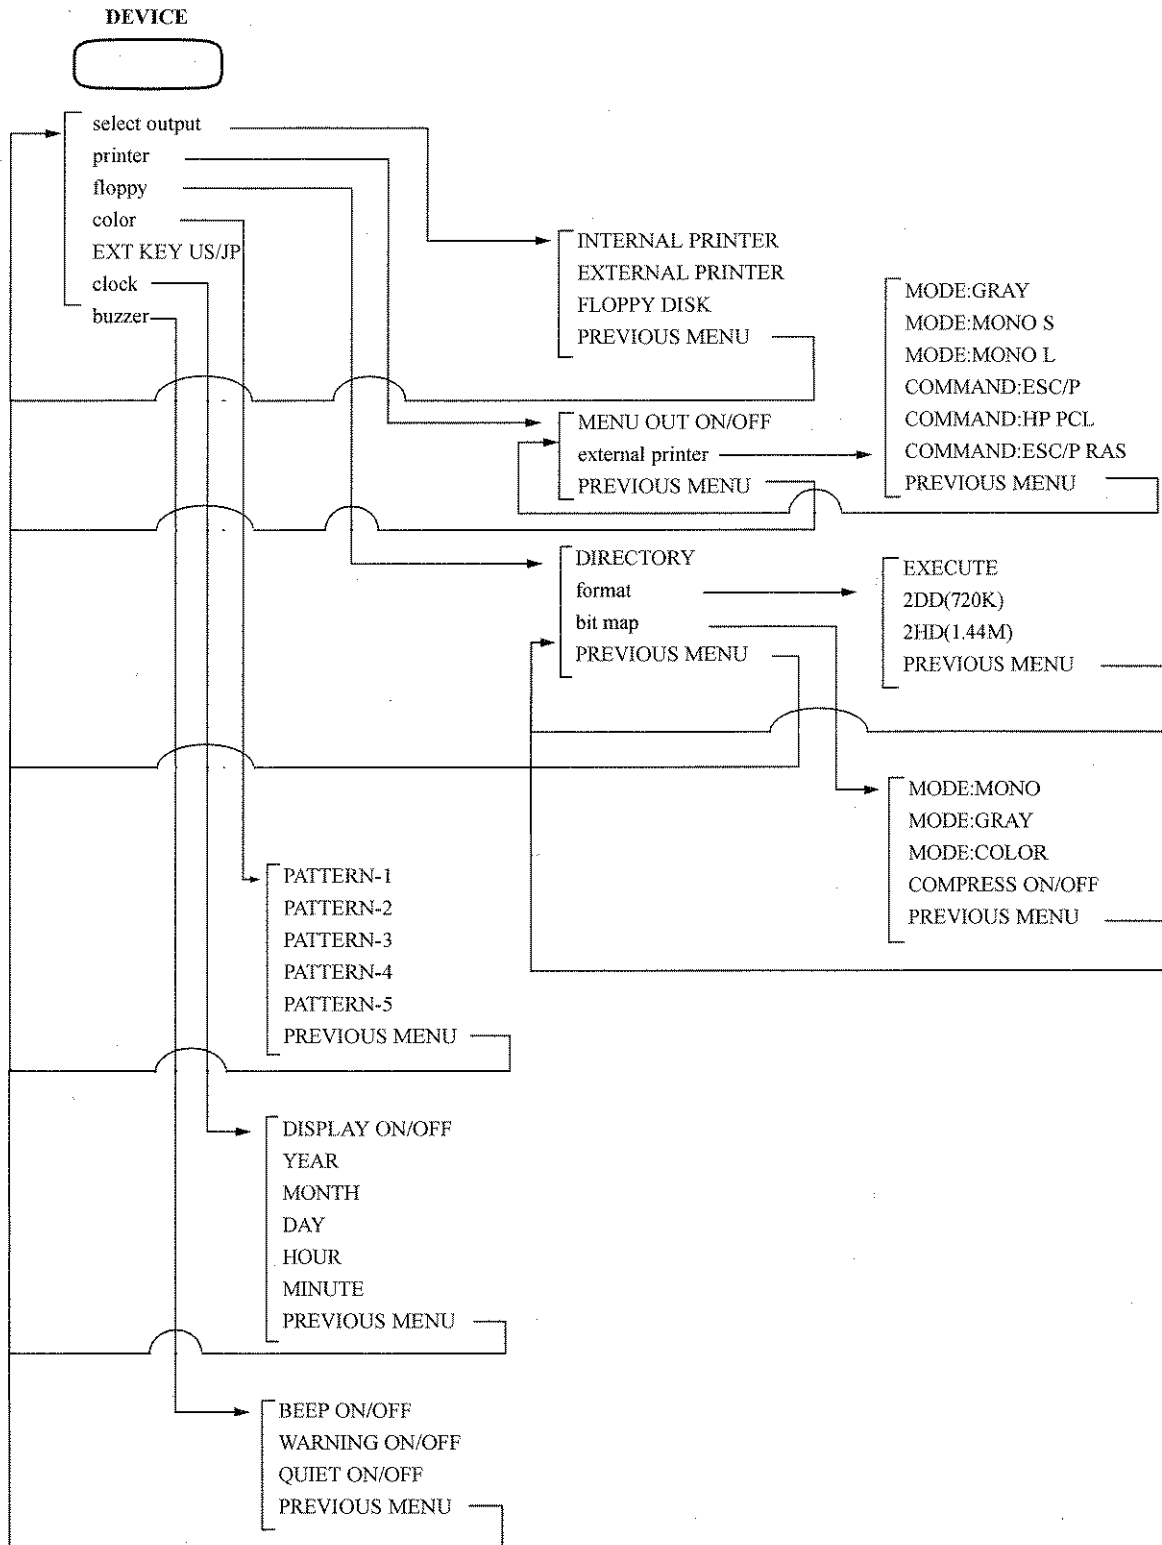



### 3.2 Menu Map


**COPY**



**FEED**



**LOCAL**



HEADER ON/OFF  
ADDRESS UP  
ADDRESS DOWN

**INSTR PRESET**



PRESET  
SELF TEST

**CAL**



CAL  $\lambda$  (Int.)  
CAL  $\lambda$  (Ext.)  
EXECUTE  
 $\lambda$  OFFSET  
LEVEL OFFSET  
RECALL OFFSET ON/OFF  
AUTO ALIGNMENT

**LABEL**



←  
→  
DELETE CHAR  
INSERT SPACE  
CLEAR LINE  
ENTER  
UNDO

### 3.3 Functional Description

This chapter describes the functions of panel key and soft key operations.

#### 3.3.1 CENTER Key

Pressing the **CENTER** key displays the CENTER menu and allows you to set the center wavelength (or frequency).

***PEAK→CENTER***

Sets the maximum peak wavelength of the displayed spectrum to the center wavelength (or frequency).

***CURSOR→CENTER***

Sets the center wavelength (or frequency) according to the value of the X cursor.

If the X cursor is not displayed, pressing this key will be ignored.

When using the single X cursor mode, the wavelength of the X cursor is set to the center wavelength (or frequency).

When using the dual X cursor mode, the wavelength at the intermediate position of each cursor is set to the center wavelength (or frequency). If an unmeasured range of wavelength is included, the range will not be displayed.

***AUTO PKC ON/OFF***

Toggles the auto peak center function on or off.

**ON:** The measured maximum peak wavelength is set to the center wavelength (or frequency) and the measurement is performed again. If the difference between the peak wavelength and the center wavelength is more than approximately 1/100 of the span, the auto peak center function will be activated.

**OFF:** Turns the auto peak center function off.

When the upper and lower screens in the dual display are both active (ACT U&L is ON), the auto peak center function is effective for the upper screen.

### 3.3.2 SPAN Key

#### 3.3.2 SPAN Key

Pressing the **SPAN** key displays the SPAN menu and allows you to set the span wavelength (or frequency).

**SPAN** Sets the span wavelength (or frequency) of the spectrum to be measured.

**START** Sets the start wavelength (the wavelength on the left side of the screen) (or frequency) of the spectrum to be measured.

**STOP** Sets the stop wavelength (the wavelength on the right side of the screen) (or frequency) of the spectrum to be measured.

**CURSOR SPAN** Sets the wavelength (or frequency) range of the spectrum to be measured into the area sandwiched by the two X cursors. The center wavelength (or frequency) will be set at the center position of the two X cursors.

**FULL SPAN** Sets the wavelength (or frequency) range of the spectrum to be measured to the maximum (1100 nm). The center wavelength will be changed to 1150 nm.(338.0013 THz)

**WAVE/FREQ nm/THz** The horizontal axis is changed to the wavelength or frequency.  
nm: Sets the spectrum horizontal axis to the wavelength.  
THz: Sets the spectrum horizontal axis to the frequency.

### 3.3.3 REF LEVEL Key

Pressing the **REF LEVEL** key allows display of the REF LEVEL menu and allows you to set the reference level.

**PEAK→REF LEVEL**

Sets and displays the reference level again so that the peak level of the currently displayed spectrum is located at a height covering approximately 95% of the screen.

**CURSOR→REF LEVEL**

Sets and displays the position of the Y cursor as the reference level.

**MAX HOLD→CURRENT**

The MAX HOLD waveform is changed to Current.

**MIN HOLD→CURRENT**

The MIN HOLD waveform is changed to Current.

**MAX HOLD ON/OFF**

Toggles the MAX HOLD function on or off.

ON: Displays a spectrum whose measurement points have the maximum level among the sweeps performed up to this time.

OFF: Turns the MAX HOLD function off.

**MIN HOLD ON/OFF**

Toggles the MIN HOLD function on or off.

ON: Displays a spectrum whose measurement points have the minimum level among the sweeps performed up to this time.

OFF: Turns the MIN HOLD function off.

**AUTO RELV ON/OFF**

Toggles the function for setting the optimum reference level for each measurement to the input signal on or off.

ON: Displays the reference level automatically optimized for each sweep.

OFF: Turns off the function for automatically setting the reference level.

---

**CAUTION** *The contents indicated by the cursor are changed when MIN HOLD or MAX HOLD is turned on. For more information, refer to Section 5.6, "Cursor Modes and Explanation for Displayed Data"*

---

### 3.3.4 LEVEL SCALE Key

#### 3.3.4 LEVEL SCALE Key

Pressing the **LEVEL SCALE** key displays the LEVEL SCALE menu and allows you to set the level scale.

##### **LVL SCALE LIN/LOG**

Toggles the function of the level scale between linear and logarithmic modes.

The graduation scale on the display can be changed only when the display is set to the log mode.

LIN: Displays the level scale linearly.

LOG: Displays the level scale logarithmically.

When the level scale is set to log mode, press the **LEVEL SCALE** key and enter a scale value using the numeric keys so that the scale can be set in steps of 0.1 dB/div.

##### **10dB/D**

The grid is displayed at 10 dB intervals.

##### **5dB/D**

The grid is displayed at 5 dB intervals.

##### **2dB/D**

The grid is displayed at 2 dB intervals.

##### **1dB/D**

The grid is displayed at 1 dB intervals.

##### **0.5dB/D**

The grid is displayed at 0.5 dB intervals.

##### **0.2dB/D**

The grid is displayed at 0.2 dB intervals.

##### **0.1dB/D**

The grid is displayed at 0.1 dB intervals.

### 3.3.5 RESOLUTION Key

Pressing the **RESOLUTION** key displays the RESOLUTION menu.

The following seven types of resolution can be set. Each resolution can be achieved by changing the slit width in the spectroscope.

<i>0.01nm</i>	The wavelength resolution is set to 0.01 nm.
<i>0.02nm</i>	The wavelength resolution is set to 0.02 nm.
<i>0.05nm</i>	The wavelength resolution is set to 0.05 nm.
<i>0.1nm</i>	The wavelength resolution is set to 0.1 nm.
<i>0.2nm</i>	The wavelength resolution is set to 0.2 nm.
<i>0.5nm</i>	The wavelength resolution is set to 0.5 nm.

### 3.3.6 SWEEP MODE Key

#### 3.3.6 SWEEP MODE Key

Pressing the **SWEEP MODE** key displays the SWEEP MODE menu. (Refer to 5.1 Measurement Modes.)

**NORMAL** Selects NORMAL in the sweep mode.  
This is selected when a normal signal is measured at high speeds.

**ADAPTIVE** Selects ADAPTIVE in the sweep mode.  
Measures signals which require relatively high sensitivity at relatively high speeds. This mode is also used to measure optical signals from pulsing emission in sync with an external signal.

**HI-SENS1** Selects HI-SENS1 in the sweep mode.  
Used to make measurements at high sensitivity.

**HI-SENS2** Selects HI-SENS2 in the sweep mode.  
Used to make measurements at a higher sensitivity than HI-SENSE1.

**HI DYNAMIC1** Selects HI DYNAMIC1 in the sweep mode.  
This is selected when a wide dynamic range must be measured by making the stray light level (of the internal optical system) lower than the ADAPTIVE.

**HI DYNAMIC2** Selects HI DYNAMIC2 in the sweep mode.  
Used to make measurements at a higher sensitivity than HI DYNAMIC1.

**PULSE** Selects PULSE in the sweep mode.  
This is selected when the spectrum in pulse emission status is measured without using an external synchronizing signal.  
The internal peak hold circuit performs the measurement after GATE TIME has been set.

**parameter** Sets the following conditions when ADAPTIVE or PULSE is selected in the sweep mode.

**SYNC HI/LOW** The response speed of the internal amplifier is switched when performing pulse synchronizing measurement in accordance with an external synchronizing signal using the GATE MEAS INPUT terminal (be sure to set the sweep mode to ADAPTIVE).

**HI:** The response of the inner amplifier will become faster. Sampling is performed using the timing previously set by DELAY and EDGE RISE/FALL.

**LOW:** The response of the inner amplifier will be returned to the normal speed. Sampling is performed using the HIGH level of an external synchronizing signal.

**DELAY** If SYNC HI mode is turned on when making an external synchronizing measurement using the GATED MEAS INPUT terminal,

sets the sampling timing using the delay time from the edge of the external synchronizing signal.

***EDGE RISE/FALL***

If SYNC HI mode is turned on when making an external synchronizing measurement using the GATED MEAS INPUT terminal, selects the sampling timing trigger.

RISE: The edge of trigger will rise.

FALL: The edge of trigger will fall.

***GATE TIME***

Sets the gate time for measurement when PULSE is selected in the sweep mode.

***PREVIOUS MENU***

Returns to the previous soft key menu.



## 3.3.7 AVG Key

## 3.3.7 AVG Key

Pressing the **AVG** key displays the AVG menu. (Refer to Section 5.2, "Average Function.")

<i>point average</i>	Average is performed after the data has been measured the specified number of times for each measurement point.
<i>1(OFF)</i>	Turns the average function off.
<i>2</i>	Sets the number of averaging processes to 2.
<i>4</i>	Sets the number of averaging processes to 4.
<i>8</i>	Sets the number of averaging processes to 8.
<i>16</i>	Sets the number of averaging processes to 16.
<i>32</i>	Sets the number of averaging processes to 32.
<i>64</i>	Sets the number of averaging processes to 64.
<i>PREVIOUS MENU</i>	Returns to the previous soft menu.
<i>sweep average</i>	Performs the averaging of the measurement data after the measurements are taken the number of averaging times.
<i>1(OFF)</i>	Turns the average function off.
<i>2</i>	Sets the number of averaging processes to 2.
<i>4</i>	Sets the number of averaging processes to 4.
<i>8</i>	Sets the number of averaging processes to 8.
<i>16</i>	Sets the number of averaging processes to 16.
<i>32</i>	Sets the number of averaging processes to 32.
<i>64</i>	Sets the number of averaging processes to 64.
<i>PREVIOUS MENU</i>	Returns to the previous soft menu.
<i>smoothing</i>	Corrects the measurement data at the specified measurement point using measurement data before and after that point (moving average).
<i>1(OFF)</i>	Turns the smoothing function off.
<i>3</i>	Performs a moving average using three points.
<i>5</i>	Performs a moving average using five points.

<i>7</i>	Performs a moving average using seven points.
<i>9</i>	Performs a moving average using nine points.
<i>11</i>	Performs a moving average using eleven points.
<i>PREVIOUS MENU</i>	Returns to the previous soft menu.

### 3.3.8 AUTO Key

Pressing the **AUTO** key displays the AUTO menu.

Automatically sets optimum measurement conditions according to the input signal.

**START** Executes the AUTO function.

**ABORT** Terminates the AUTO function.

### 3.3.9 SINGLE Key

Pressing the **SINGLE** key allows one measurement operation to be performed. The LED on the **SINGLE** key lights up during measurement. When the measurement is completed, the LED turns off.

Pressing the **SINGLE** key during measurement causes the current measurement to be interrupted and starts a new measurement.

### 3.3.10 REPEAT Key

Pressing the **REPEAT** key causes the measurement operation to be performed repeatedly. During repeat measurements, the LED on the **REPEAT** key lights up until the **SINGLE** key or the **STOP** key is pressed. Pressing the **REPEAT** key during measurement causes the current measurement to be interrupted and starts a set of new repeated measurements.

### 3.3.11 STOP Key

Pressing the **STOP** key causes the measurement operation to be stopped. The measurement operation is stopped immediately after the **STOP** key is pressed. The LED on the **SINGLE** key or the LED on the **STOP** key turns off. When pressing the **STOP** key to stop measurement, the data displayed at that time will be retained as is.

### 3.3.12 NORMALIZE LOSS/TRANS Key

#### 3.3.12 NORMALIZE LOSS/TRANS Key

Pressing the **NORMALIZE LOSS/TRANS** key displays the **NORMALIZE** menu. (Refer to Section 5.5, "Auto-panning and Auto-zooming Functions").

**PEAK NORMALIZE** Selects the mode for normalizing the measurement data at the maximum value.

**LOSS** Selects the mode for calculating and displaying the loss characteristics. Normalizes the measurement data to the reference data saved in the memory using the same (and corresponding) wavelengths between the current spectrum and the spectrum data saved to memory.

---

*NOTE: LINEAR display is impossible under this mode.*

---

**TRANS** Selects the mode for calculating and displaying the transparency characteristics. Normalizes the measurement data to the reference data saved in the memory using the same (and corresponding) wavelengths between the current spectrum and the spectrum data saved to memory.

**SAVE REF DATA** Saves the current measurement data as reference data in memory.

**SAVE MEAS 1** Saves the current measurement data in memory 1.

### 3.3.13 APPLICATION Key

Pressing the **APPLICATION** key displays the **APPLICATION** menu.

---

**NOTE:** Parameters marked with (#) also apply to *opt.amp*, *wdm* and *wdm monitor*.

---

<i>spectral width</i>	Selects the function for calculating the pulse duration. Refer to Section 5.3.1, "Calculating the Spectral Width."
<b>PEAK-THRESHOLD</b>	Selects the mode for calculating the pulse duration to the maximum value or noise level according to the threshold method.
<b>ENVELOPE</b>	Selects the mode for calculating the pulse duration according to the envelope method.
<b>RMS</b>	Selects the mode for calculating the pulse duration according to the RMS method.
<b>PEAK RMS</b>	Selects the mode for calculating the pulse duration according to the peak RMS method.
<b>Xnm LEVEL</b>	Selects the mode for calculating the ratio of the peak level to the level of a wavelength separated by a specified wavelength width as centered approximately the maximum value wavelength.
<i>parameter</i>	Displays the operation parameter menu related to spectral widths.
<b>THRESHOLD LVL1(dB)</b>	Sets the level threshold used in the <b>PEAK THRESHOLD</b> or <b>ENVELOPE</b> method. (The initial value is 3dB.)
<b>THRESHOLD LVL2(dB)</b>	Sets the level threshold from the maximum peak level when calculating the numbers of peaks. (The initial value is 20dB.)
<b>K</b>	Sets the coefficient multiplied to the calculated pulse duration. (The initial value is 1.0.)
<b>Kr(RMS)</b>	Sets the coefficient multiplied to the pulse duration calculated by the <b>RMS</b> method or the <b>PEAK RMS</b> method. (The initial value is 2.3548.)
<b>WIDTH</b>	Sets the width for calculating the level ratio in the <b>Xnm-LEVEL</b> calculation.
<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
<b>OFF</b>	Turns the half band width calculation function off.

3.3.13 APPLICATION Key

<i>notch width</i>	Selects the notch width calculation function. Refer to Section 5.3.2, "Notch Width."
<i>XdB WIDTH</i>	Calculates the notch width separated from the threshold level.
<i>Xnm LEVEL</i>	Calculates the level ratio separated from the wavelength width.
<i>parameter</i>	Displays the operation parameter menu related to notch width.
<i>LEVEL</i>	Sets the level ratio.
<i>WIDTH</i>	Sets the wavelength width.
<i>PREVIOUS MENU</i>	Returns to the previous soft key menu.
<i>OFF</i>	Turns the notch width calculation function off.
<i>opt.amp</i>	Changes to the menu for calculating the gain/noise index of the EDFA. For information on how to operate this function, refer to Section 5.4, "Gain, NF and SNR."
<i>MODE SNG/WDM</i>	Switches between single wave and wavelength multiplexing in the calculation result display mode. SNG: Selects a single signal. WDM: Selects a wavelength division multiplexing (WDM) signal.
<i>parameter</i>	Switches the current menu to the menu for setting the calculation parameter.
↓	Moves the setting parameter downward by one position.
↑	Moves the setting parameter upward by one position.
←	Moves the setting parameter to the left by one position.
→	Moves the setting parameter to the right by one position.
<i>CLOSE</i>	Closes the window for setting the calculation parameter.
<i>NF Select</i>	Sets whether only the term of the beat noise between the signal light and spontaneous emission light (s-sp) is used, or four terms (total) consisting of the beat noise between the signal light and spontaneous emission light, the beat noise between spontaneous emission lights, the shot noise of signal light, and the shot noise of spontaneous emission light are used when calculating the noise figure.

<b>WDM ASE Method (#)</b>	Sets whether or not to automatically calculate ASE when set to WDM mode.
<b>ASE Fitting (#)</b>	Controls whether the Gaussian fitting is used, the measured data stored in memory 3 is used, or data is manually entered to calculate the ASE level. When "WDM ASE METHOD" is set to "AUTO OFF."
<b>Threshold Level (#)</b>	The value is calculated only when the signal level is between the peak level and the level the specified value below the peak level.
<b>Masked Span (#)</b>	Sets the width to be masked around the center of the signal light in the fitting process.
<b>Fitting Span (#)</b>	Sets the target wavelength used in the fitting process when calculating the ASE level.
<b>Method (#)</b>	Sets whether or not SPE DIV Mode is turned on. SPE DIV Mode cancels errors caused by stray light, input signal's amplified spontaneous emission, side mode, and so on.
<b>NF K</b>	Sets the coefficient for the noise figure calculated. This parameter is used when the correction is required other than input/output loss.
<b>Filter <math>\Delta\lambda</math></b>	Sets the effective optical filtering width of the optical amplifier output which is used for the noise figure calculation when NF SELECT is set to total. When set to 0, the NF is calculated including the terms "Beat noise between the optical signal and the spontaneous emission" and "Optical signal shot noise."
<b>Manual ASE Level (#)</b>	Sets the ASE level when ASE Fitting is set to Manual Mode.
<b>Pin LOSS</b>	Sets the differences between the optical signal level input into the instrument and the optical signal level actually input into the optical amplifier.
<b>Pout LOSS</b>	Sets the differences between the output optical signal level of the optical amplifier input into the instrument and the optical signal level actually output from the optical amplifier.
<b>NEXT PAGE</b>	Moves the signal list display in WDM to the next page.
<b>PREVIOUS PAGE</b>	Moves the signal list display in WDM to the previous page.
<b>SAVE Pin→REF DATA</b>	Saves an EDFA input signal waveform in reference memory.
<b>SAVE MEM 3</b>	Saves the waveform data in memory 3.

3.3.13 APPLICATION Key

<i>OFF</i>	Exits from the EDFA evaluation mode.
<i>wdm</i>	Selects the WDM analysis mode.
<i>MULTI PEAK</i>	Selects MULTI PEAK in the list display mode.
<i>SNR</i>	Selects SNR in the list display mode. For information on how to operate this function, refer to Section 5.4, "Gain, NF and SNR."
<i>RELATIVE</i>	Selects RELATIVE in the list display mode.
<i>ITU GRID</i>	Selects ITU-GRID in the list display mode.
<i>parameter</i>	Switches the current menu to the menu for setting the calculation parameter.
↓	Moves the setting parameter downward by one position.
↑	Moves the setting parameter upward by one position.
←	Moves the setting parameter to the left by one position.
→	Moves the setting parameter to the right by one position.
<i>CLOSE</i>	Closes the window for setting the calculation parameter.
<i>WDM ASE Method (#)</i>	Sets whether or not an ASE interpolation is automatically performed.
<i>ASE Fitting (#)</i>	Controls whether the Gaussian fitting is used, the measured data stored in memory 3 is used, or data is manually entered to calculate the ASE level. When "WDM ASE METHOD" is set to "AUTO OFF."
<i>Threshold Level (#)</i>	Sets the effective range below the peak level.
<i>Masked Span (#)</i>	Sets the width to be masked around the center of the signal light in the fitting process.
<i>Fitting Span (#)</i>	Sets the target wavelength used in the fitting process when calculating the ASE level.

<b>ASE NBW (#)</b>	<p>A parameter used to calculate the amplified spontaneous emission level (Pase) when the list display mode is set to SNR. (NBW:Noise acquisition Band Width)</p> <p>Current: The measurement spectrum is used as the amplified spontaneous emission level (Pase).</p> <p>Conversion: The amplified spontaneous emission level is calculated by assigning an arbitrary wavelength resolution to the expression shown below.</p> $\text{Pase (Calculated)} = \text{Pase (Measurement value)} \times \text{Res (Set resolution of "ASE Converted NBW")}/\text{Res (Current measurement wavelength resolution)}$
<b>ASE Converted NBW (#)</b>	<p>Sets the wavelength resolution used to calculate Pase when the ASE NBW is set to Conversion.</p>
<b>Manual ASE Level (#)</b>	<p>Sets the ASE level when ASE Fitting is set to Manual Mode.</p>
<b>GRID ref. Frequency (#)</b>	<p>Sets the reference frequency of the WDM-signal nominal frequency when the list display mode is set to ITU GRID.</p>
<b>GRID CH Spacing (#)</b>	<p>Sets the channel spacing frequency of the WDM-signal nominal frequency when the list display mode is set to ITU GRID.</p>
<b>LIST ALL ON/OFF</b>	<p>Up to 24 signals can be displayed in the list at the same time on the entire screen.</p>
<b>REFERENCE</b>	<p>Sets the reference CH No. in the list. The signal assigned to the reference CH is indicated with an inverted triangle <math>\nabla</math> on the spectrum screen.</p>
<b>OFF</b>	<p>Exits from the WDM analysis mode.</p>
<b>wdm monitor</b>	
<b>DISPLAY MONI/SPEC</b>	<p>Toggles the display mode (in the upper display area) between the Monitor graph and Spectrum.</p>
<b>GRAPH X TIME/CH</b>	<p>Toggles the monitor graph X-axis between the time and channel.</p>
<b>TBL CONT TIME/CH</b>	<p>Changes scrolling and CURRENT in the data table in combination with the <b>CURRENT SELECT</b> key.</p>
<b>data mode</b>	<p>Changes the table data mode.</p>
<b><math>\lambda</math>,f</b>	<p>Changes the table display to the wavelength (frequency) mode.</p>



3.3.13 APPLICATION Key

<i>LEVEL</i>	Changes the table display to the level mode.
<i>SNR</i>	Changes the table display to the SNR mode.
<i>PREVIOUS MENU</i>	Returns to the previous menu.
<i>absolute/relative</i>	Toggles the table display between the absolute and relative modes.
<i>ABSOLUTE</i>	Displays the table data in absolute values.
<i>INITIAL</i>	Displays the table data as changes compared to the initial value. (When X-axis represents the time, the first measurement value is the initial value for each channel.) (When X-axis represents the channel, the first channel measurement value at each specified time is the initial value.)
<i>NOMINAL</i>	Displays the table data as changes compared to the target value. When the data mode is set to $\lambda f$ , the frequency determined by GRID ref Frequency and GRID CH Spacing is the target value. When the data mode is set to LEVEL, the value set in Nominal Level is the target value. When the data mode is set to SNR, the value set in Nominal SNR is the target value.
<i>PREVIOUS MENU</i>	Returns to the previous menu.
<i>parameter</i>	Switches to the desired operation parameter menu.
↓	Shifts the parameter downwards by one position.
↑	Shifts the parameter upwards by one position.
←	Shifts the parameter to the left by one position.
→	Shifts the parameter to the right by one position.
<i>CLOSE</i>	Closes the menu used to set operation parameters.
<i>Time Interval</i>	Sets the measurement time interval.
<i>Graph All Data</i>	All data except the currently selected data is displayed in the monitor graph display area.

**ASE Fitting (#)** Sets how the ASE level is entered when WDM ASE METHOD is set to AUTO OFF: entering the ASE level after it has been calculated using the Gaussian fitting, entering the data saved in memory3 for the ASE level, or entering data manually for the ASE level.

**Threshold Level (#)** A calculation begins after the level below the peak has been recognized as an effective optical signal.

**Masked Span (#)** Sets a span that is masked around the center of the optical signal and removed from the fitting process.

**Fitting span (#)** Sets a wavelength width for the fitting process when calculating the ASE level.

**Pass/Fail enable** Sets whether or not a Pass/Fail judgment is made. If the value is judged Fail since it has exceeded the limit, the number in the table is intensified.

**Level Upper Lmt.** Sets the upper limit for each signal level when making a Pass/Fail judgment.

**Level Lower Lmt.** Sets the lower limit for each signal level when making a Pass/Fail judgment.

**SNR Lower Lmt.** Sets the lower limit for each SNR when making a Pass/Fail judgment.

**Measurement Times** Sets the number of times the measurement is repeated.

**WDM ASE Method (#)** Sets whether or not an interpolation for the ASE is automatically performed.

**ASE NBW (#)** A parameter used to calculate the amplified spontaneous emission level (Pase) when the contents of the data table is SNR. (NBW:Noise acquisition Band Width)

Current: The measurement spectrum is used as the amplified spontaneous emission level (Pase).

Conversion:

The amplified spontaneous emission level is calculated by assigning an arbitrary wavelength resolution to the expression shown below.

$$\text{Pase (Calculated)} = \text{Pase (Measurement value)} \times \text{Res (Set resolution of "ASE Converted NBW")}/\text{Res (Current measurement wavelength resolution)}$$

3.3.13 APPLICATION Key

- ASE Converted NBW (#)** Sets the wavelength resolution used to calculate Pase when the ASE NBW is set to Conversion.
- Manual ASE Level (#)** Sets the ASE level when ASE FITTING is set to Manual Mode.
- GRID ref. Frequency (#)** Sets the reference frequency of a WDM signal.
- GRID CH Spacing (#)** Sets the reference frequency of a WDM signal.
- $\lambda$  drift Lmt.** Sets the upper limit of the wavelength drift for each channel when making a Pass/Fail judgment.
- Nominal Level** Sets the target signal level for each channel of a WDM signal.
- Nominal SNR** Sets the target SNR for each channel of a WDM signal.
- CURRENT SELECT** Changes scrolling and CURRENT in the data table in combination with the TBL CONT key.

Table 3-1 Changing the Table Data Display and the Current Time or Channel

		TBL CONT	
		TIME	CH
CURRENT SELECT	ON	Changes the current time.	Changes the current channels.
	OFF	Scrolls the table data along the time axis.	Scrolls the table data along the channel axis.

The expressions CURRENT TIME and CURRENT CH refer to the data displayed in the upper display area (When Graph All Data is selected, the color of the current waveform is different from the other waveform colors.).

If the X-axis represents the time, the channel data specified by CURRENT CH is displayed as a monitor graph along the time axis.

If the X-axis represents the channel, the data specified at CURRENT TIME is displayed as a monitor graph along the channel axis.

**OFF** Turns WDM MONITOR off.

### 3.3.14 ADVANCE Key

Pressing the **ADVANCE** key displays the ADVANCE menu.

<i>peak power-mon</i>	Selects the peak power monitor function.
<i>SAMPLING POINT</i>	Sets the maximum sampling numbers in SINGLE measurement.
<i>INTERVAL TIME</i>	Sets the time interval for sampling.
<i>OFF</i>	Exits from the peak power monitor function.
<i>limit line</i>	Selects a function from the Pass/Fail function.
<i>PATTERN1</i>	Loads data from the PATTERN1 file as the limit line.
<i>PATTERN2</i>	Loads data from the PATTERN2 file as the limit line.
<i>PATTERN3</i>	Loads data from the PATTERN3 file as the limit line.
<i>PATTERN4</i>	Loads data from the PATTERN4 file as the limit line.
<i>PATTERN5</i>	Loads data from the PATTERN5 file as the limit line.
<i>LOAD PATTERN FILES</i>	Loads the limit line pattern file from a floppy disk. For information how to create the pattern file, refer to Section 5.7, "Limit Line Settings" in the technical notes.
<i>PASS/FAIL</i>	Makes a Pass/Fail judgment.
<i>OFF</i>	Exits from the limit line function.

### 3.3.15 ON/OFF Key

#### 3.3.15 ON/OFF Key

Pressing the **ON/OFF** key (in the **CURSOR** section) displays the **CURSOR** menu.

The selection of cursor displays and display formats for cursor data can be performed. (Refer to 5.6 Cursor Modes and Explanation for Displayed Data.)

<b>NORMAL</b>	Sets the cursor call mode to the <b>NORMAL</b> .
<b><math>\Delta</math>MODE</b>	Sets the cursor call mode to the <b><math>\Delta</math>MODE</b> .
<b>2ND PEAK</b>	Sets the cursor call mode to <b>2ND PEAK</b> . X cursor 1 moves to the highest peak and X Cursor 2 moves to the second highest peak.
<b>POWER</b>	Sets the cursor call mode to <b>POWER</b> . Displays the total power of the signal section between the two X Cursors.
<b>PEAK TO PEAK</b>	Sets the cursor call mode to <b>PEAK TO PEAK</b> . One X Cursor moves to the maximum value, and the other X Cursor moves to the minimum value.
<b>LEFT PEAK</b>	Moves X Cursor 2 over the next peak on the left side. In addition, if Y Cursor 2 is displayed, only the peaks whose levels are above the Y Cursor 2 level are targeted.
<b>RIGHT PEAK</b>	Moves X Cursor 2 over the next peak on the right side. In addition, if Y Cursor 2 is displayed, only the peaks whose levels are above the Y Cursor 2 level are targeted.

#### 3.3.16 $\lambda$ 1 Key

Pressing the  $\lambda$ 1 key displays the first cursor perpendicular to the wavelength axis. Pressing the  $\lambda$ 1 key again erases the cursor.

#### 3.3.17 $\lambda$ 2 Key

Pressing the  $\lambda$ 2 key displays the second cursor perpendicular to the wavelength axis. Pressing the  $\lambda$ 2 key again erases the cursor.

#### 3.3.18 L1 Key

Pressing the **L1** key displays the first cursor horizontal to the wavelength axis. Pressing the **L1** key again erases the cursor.

#### 3.3.19 L2 Key

Pressing the **L2** key displays the second cursor horizontal to the wavelength axis. Pressing the **L2** key again erases the cursor.

### 3.3.20 CONTROL Key

Pressing the **CONTROL** key displays the CONTROL menu.

<b>DUAL ON/OFF</b>	Toggles the dual screen display function for the upper and the lower screens on or off. ON: Displays the dual upper and lower screens. OFF: Displays only one screen.
<b>S.IMPOSE ON/OFF</b>	Toggles the function for superimposing display on or off. ON: Displays by superimposing. OFF: Turns the function for superimposing display off.
<b>multi trace</b>	Turns the multi-trace function on. The current trace is saved as No. 1. The color of the current trace is displayed in yellow. The colors of the traces other than the current trace are displayed in the order of green, blue, sky blue and red.
<b>TRACE MAX</b>	Sets the maximum trace number (1 to 32).
<b>NEXT</b>	The current trace is shifted to the next number.
<b>PREV</b>	The current trace is shifted to the previous number.
<b>AUTO TRAC ON/OFF</b>	Toggles the auto-trace function on or off. When the auto-trace function is turned on, the current trace number is automatically incremented for each sweep.
<b>DELETE CURRENT</b>	Deletes the current trace.
<b>DELETE ALL</b>	Deletes all traces.
<b>OFF</b>	Turns the multi-trace function off. Only the current trace is left undeleted.
<b>GRID ON/OFF</b>	Toggles the grid display function on or off. Displays and erases the grid lines within the data display frame.
<b>ACT U&amp;L ON/OFF</b>	Toggles the function used to update the upper and lower screens (for each measurement in the dual screen mode) on or off. ON: The upper and lower screens are updated for each measurement. OFF: Only the upper screen is updated.
<b>X-CHANGE UPR/LOW</b>	Exchanges between the upper and lower screens only in Dual Screen Mode.
<b>sampling point</b>	Sets the sampling point within the wavelength range.

3.3.20 CONTROL Key

<i>101</i>	Sets the sampling point within the wavelength range to 101 points.
<i>201</i>	Sets the sampling point within the wavelength range to 201 points.
<i>501</i>	Sets the sampling point within the wavelength range to 501 points.
<i>1001</i>	Sets the sampling point within the wavelength range to 1001 points.
<i>2001</i>	Sets the sampling point within the wavelength range to 2001 points.
<i>5001</i>	Sets the sampling point within the wavelength range to 5001 points.
<i>10001</i>	Sets the sampling point within the wavelength range to 10001 points.
<i>AUTO ON/OFF</i>	Toggles the auto-sampling point function on or off. ON: Automatically sets the sampling points according to the span and resolution. The character "A" is affixed to the screen annotation for the number of sampling points. OFF: Turns the auto-sampling point function off.

**3.3.21 SAVE Key**

Pressing the **SAVE** key displays the **SAVE** menu. (Refer to Section 2.3.4, "Saving or Reading Data.")

<b>SAVE REF DATA</b>	Stores the current measurement data into memory as reference data. The reference data is used with <b>NORMALIZE LOSS/TRANS</b> . In addition, the reference data is used for the spectrum of the input signal in the <b>opt amp</b> function (to calculate the gain and NF of an optical amplifier).
<b>SAVE MEAS 1</b>	Saves the current measurement data into memory 1. However, the data created using the <b>Peak Normalized</b> , <b>Peak Power Monitor</b> , <b>Loss</b> or <b>Trans</b> function cannot be saved.
<b>SAVE MEAS 2</b>	Saves the current measurement data into memory 2.
<b>SAVE MEAS 3</b>	Saves the current measurement data into memory 3. This trace data is used as a fitting function when <b>ASE</b> fitting is set to <b>MEM-3</b> .
<b>save meas data</b>	Moves to the save menu for the measurement data.
<b>SAVE</b>	Saves the file name selected.
<b>DELETE</b>	Deletes the file name selected.
<b>RECOVER</b>	Recovers the file name deleted just before recovering.
<b>name</b>	Moves to the menu that inputs the file name.
←	Moves the input cursor to the left by one character.
→	Moves the input cursor to the right by one character.
<b>NAME CLEAR</b>	Clears the input memory name (file name).
<b>ENTER</b>	Selects characters from the character menu.
<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
<b>EXIT</b>	Returns to the waveform display mode.
<b>SAVE MEM/FDD</b>	Switch the media for saving the data between memory and <b>FDD</b> . MEM: Saves the data into memory. FDD: Saves the data to the floppy disk drive.



3.3.22 RECALL Key

**3.3.22 RECALL Key**

Pressing the **RECALL** key displays the RECALL menu.

<i>RECALL REF DATA</i>	Recalls data from the reference data memory.
<i>RECALL MEAS 1</i>	Recalls data from memory MEAS1.
<i>RECALL MEAS 2</i>	Recalls data from memory MEAS2.
<i>RECALL MEAS 3</i>	Recalls data from memory MEAS3.
<i>recall meas data</i>	Moves to the recall menu for the measurement data.
<i>RECALL</i>	Recalls from the selected file name.
<i>EXIT</i>	Returns to the waveform display mode.
<i>RECALL MEM/FDD</i>	Switch the media for recalling data between memory and FDD. MEM: Data is loaded from memory. FDD: Data is loaded from the floppy disk drive.

### 3.3.23 DEVICE Key

Pressing the **DEVICE** key displays the DEVICE menu.

<i>select output</i>	Selects the output device.
<b>INTERNAL PRINTER</b>	Selects the internal thermal printer as the output device.
<b>EXTERNAL PRINTER</b>	Selects the external printer as the output device.
<b>FLOPPY DISK</b>	Selects the floppy disk as the output device.
<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
<i>printer</i>	Sets the printer parameter.
<b>MENU OUT ON/OFF</b>	Toggles the soft key menu on (to output) or off (not to output). ON: Outputs the soft key menu on the right side of the screen when the printer is outputting. OFF: Does not output the soft key menu.
<i>external printer</i>	Sets the parameter for external printer output.
<b>MODE:GRAY</b>	Prints in 4 gradations.
<b>MODE:MONO S</b>	Prints in 2 gradations of white and black in small size.
<b>MODE:MONO L</b>	Prints in 2 gradations of white and black in large size.
<b>COMMAND:ESC/P</b>	Outputs according to ESC/P.
<b>COMMAND:HP PCL</b>	Outputs according to HP PCL.
<b>COMMAND:ESC/P RAS</b>	Outputs according to ESC/P RAS.
<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
<i>floppy</i>	Sets the parameter for outputting data to the floppy disk.
<b>DIRECTORY</b>	Used to display the directory information of all the files in the floppy disk.
<i>format</i>	Sets the format parameter.
<b>EXECUTE</b>	Executes the format.

3.3.23 DEVICE Key

	<b>2DD(720K)</b>	Selects format capacity 2DD-720K.
	<b>2HD(1.44M)</b>	Selects format capacity 2HD-1.44M.
	<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
<b>bit map</b>		Records the display screen using the bitmap.
	<b>MODE:MONO</b>	Records in 2 gradation of white and lack.
	<b>MODE:GRAY</b>	Records in gray scale.
	<b>MODE:COLOR</b>	Records in 256 colors.
	<b>COMPRESS ON/OFF</b>	Toggles the compression function of the bitmap on or off.
	<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
	<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
<b>color</b>		Selects the color pattern.
	<b>PATTERN-1</b>	Selects color pattern 1.
	<b>PATTERN-2</b>	Selects color pattern 2.
	<b>PATTERN-3</b>	Selects color pattern 3.
	<b>PATTERN-4</b>	Selects color pattern 4.
	<b>PATTERN-5</b>	Selects color pattern 5.
	<b>PREVIOUS MENU</b>	Returns to the previous soft key menu.
	<b>EXT KEY US/JP</b>	Toggles the keyboard between the US layout (104) and the Japanese layout (109).
<b>clock</b>		Sets the real time clock. (Refer to Section 2.3.3, "Setting Date/Time.")
	<b>DISPLAY ON/OFF</b>	Toggles on (to display) or off (not to display) the date display. ON: Displays the date. OFF: Does not display the date.
	<b>YEAR</b>	Sets the year.
	<b>MONTH</b>	Sets the month.

<i>DAY</i>	Sets the day.
<i>HOUR</i>	Sets the hour.
<i>MINUTE</i>	Sets the minute. At the same time it sets the seconds to 00.
<i>PREVIOUS MENU</i>	Returns to the previous soft key menu.
<i>buzzer</i>	Sets the conditions for sounding the buzzer. Buzzer sounds include two types: one sound that is activated when the panel keys are pressed and another sound that is activated when measurement conditions, etc. are set illegally.
<i>BEEP ON/OFF</i>	Sets whether to beep when the panel keys are pressed. ON:     Beeps when the panel keys are pressed. OFF:    Does not beep when the panel keys are pressed.
<i>WARNING ON/OFF</i>	Sets whether the warning buzzer is sounded or not when error occurs. ON:     Sounds the warning buzzer when error occurs. OFF:    Does not sound the warning buzzer when error occurs.
<i>QUIET ON/OFF</i>	Toggles on or off the function of decreasing buzzer sound volume. ON:     Decreases the sound volume of the buzzer. OFF:    Does not control the sound volume of the buzzer.
<i>PREVIOUS MENU</i>	Returns to the previous soft key menu.

### 3.3.24 COPY Key

#### 3.3.24 COPY Key

Pressing the **COPY** key outputs the data to be copied to the output device set by Select Output. (Refer to Section 2.3.5, "Outputting Data (Hard Copy).")

#### 3.3.25 FEED Key

Pressing the **FEED** key performs paper feed in the internal printer.

#### 3.3.26 LOCAL Key

**HEADER ON/OFF**

Turns ON (to add)/OFF (not to add) the header when outputting the GP-IB data.

ON: Adds the header when outputting data.

OFF: Does not add the header when outputting data.

**ADDRESS UP**

Increments the GPIB address by 1.

**ADDRESS DOWN**

Decrements the GPIB address by 1.

#### 3.3.27 INSTR PRESET Key

**PRESET**

Sets the panel setting conditions to the initial setting status.

**SELF TEST**

Conducts a self test and displays the results after approximately 90 seconds.

### 3.3.28 CAL Key

(Refer to Section 2.2.4, "Alignment" and Section 2.2.5, "Calibration.")

<b><i>CAL <math>\lambda</math> (Int)</i></b>	Calibrates the wavelength using the optional self-contained light source.
<b><i>CAL <math>\lambda</math> (Ext)</i></b>	Calibrates the wavelength using the external laser light source as the calibration light source.
<b><i>EXECUTE</i></b>	Executes the calibration operation.
<b><i><math>\lambda</math> OFFSET</i></b>	Inputs the offset value of the wavelength.
<b><i>LEVEL OFFSET</i></b>	Inputs the offset value of the level.
<b><i>RECALL OFFSET ON/OFF</i></b>	Toggles the function used to load wavelength and level offset data (before a data file or panel information is loaded) on or off. ON: Recalls the offset parameter. OFF: Does not recall the offset parameter.

---

***NOTE:*** When the offset data is not enabled, please input 0 to the  $\lambda$  offset and the LEVEL OFFSET.

---

***AUTO ALIGNMENT*** This function adjusts the optical axis of the monochromator used with the optical spectrum analyzer.

---

***CAUTION:*** Prior to operating this instrument immediately after having transported it with fierce vibrations, or operating this instrument in a place having abrupt temperature changes, be sure to warm up the instrument and then perform the ***AUTO ALIGNMENT*** function in advance.

---

3.3.29 LABEL Key

**3.3.29 LABEL Key**

(Refer to Section 2.3.1, "Entering Label Data.")

←	Moves the input cursor in the label to the left by one character.
→	Moves the input cursor in the label to the right by one character.
<i>DELETE CHAR</i>	Deletes a character at the input cursor position.
<i>INSERT SPACE</i>	Inserts a space at the input cursor position.
<i>CLEAR LINE</i>	Clears all data in the label input buffer.
<i>ENTER</i>	Sets the input character selected by the character menu.
<i>UNDO</i>	Recovers the label data to the status before the key is pressed.

### 3.4 List of Settings

#### 3.4.1 Defaults Configuration Values

The center wavelength and span wavelength along the horizontal axis are calculated into the center frequency and span frequency, respectively.

Table 3-2 Default Settings

Item	Default	Minimum value	Maximum value	Setting resolution	Backup	File save
Center wavelength (nm)	1150	600	1700	0.001	<input type="radio"/>	<input type="radio"/>
Span wavelength (nm)	1100	0.2	1100	0.1	<input type="radio"/>	<input type="radio"/>
Auto peak center	OFF	-	-	-	<input type="radio"/>	<input type="radio"/>
Spectral horizontal axis	nm	-	-	-	<input type="radio"/>	<input type="radio"/>
Reference level (dBm)	0	-90	30	0.1	<input type="radio"/>	<input type="radio"/>
Reference level (LIN)	1mW	1pW	1000mW	0.1	<input type="radio"/>	<input type="radio"/>
Minimum hold	OFF	-	-	-	<input type="radio"/>	<input type="radio"/>
Maximum hold	OFF	-	-	-	<input type="radio"/>	<input type="radio"/>
Reference auto	OFF	-	-	-	<input type="radio"/>	<input type="radio"/>
LIN/LOG	LOG	-	-	-	<input type="radio"/>	<input type="radio"/>
Level scale	10dB/DIV	0.1	10	0.1	<input type="radio"/>	<input type="radio"/>
AUTO measurement	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Point average	OFF	1	64	1	<input type="radio"/>	<input type="radio"/>
Sweep average	OFF	1	64	1	<input type="radio"/>	<input type="radio"/>
Smoothing	OFF	1	11	2	<input type="radio"/>	<input type="radio"/>
Sweep mode	NORMAL	-	-	-	<input type="radio"/>	<input type="radio"/>
Gate Time(sec)	0.01	0	1	0.001	<input type="radio"/>	<input type="radio"/>
SYNC	Low	-	-	-	<input type="radio"/>	<input type="radio"/>
DELAY( $\mu$ sec)	10	0	1000	0.1	<input type="radio"/>	<input type="radio"/>
EDGE	RISE	-	-	-	<input type="radio"/>	<input type="radio"/>
Wavelength resolution (nm)	0.2	0.01	0.5	-	<input type="radio"/>	<input type="radio"/>
Cursor	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>



## 3.4.1 Defaults Configuration Values

Table 3-2 Default Settings

Item	Default	Minimum value	Maximum value	Setting resolution	Backup	File save
Cursor data	NORMAL	-	-	-	<input type="radio"/>	<input type="radio"/>
Dual screen display	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Superimpose mode	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Multi trace	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Trace max	8	1	32	1	<input type="radio"/>	<input type="radio"/>
Current trace No.	1	1	32	1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Auto trace	ON	-	-	-	<input type="radio"/>	<input type="radio"/>
Grid	ON	-	-	-	<input type="radio"/>	<input type="radio"/>
Sampling point	501	101	10001 Note 1	-	<input type="radio"/>	<input type="radio"/>
Auto sample	OFF	-	-	-	<input type="radio"/>	<input type="radio"/>
Peak normalize	OFF	-	-	-	<input checked="" type="checkbox"/>	<input type="radio"/>
Power monitor	OFF	-	-	-	<input type="radio"/>	<input type="radio"/>
Power monitor times	101	11	1001	1	<input type="radio"/>	<input type="radio"/>
Power monitor interval (sec)	0.5	0.5	3600	0.1	<input type="radio"/>	<input type="radio"/>
Limit line	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Spectral width	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Spectral width type	pk-XdB	-	-	-	<input type="radio"/>	<input type="radio"/>
THRESHOLD LVL1 (dB)	3	-59.9	59.9	0.01	<input type="radio"/>	<input type="radio"/>
THRESHOLD LVL2 (dB)	20	0.1	99.9	0.01	<input type="radio"/>	<input type="radio"/>
K Parameter (RMS, Peak RMS)	1	0.1	100	0.01	<input type="radio"/>	<input type="radio"/>
Kr(RMS)	2.3548	1	10	0.0001	<input type="radio"/>	<input type="radio"/>
Spectral width width(nm)	1	0.01	100	0.01	<input type="radio"/>	<input type="radio"/>
Notch width	OFF	-	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Notch width level(dB)	3	-59.9	59.9	0.01	<input type="radio"/>	<input type="radio"/>
Notch width width(nm)	1	0.01	100	0.01	<input type="radio"/>	<input type="radio"/>

Note 1: Up to 2001 points when the multi-trace function is turned on

Table 3-2 Default Settings

Item	Default	Minimum value	Maximum value	Setting resolution	Backup	File save
Opt AMP	OFF	-	-	-	×	×
Opt AMP MODE	Single	-	-	-	○	○
NF(s-sp) or NF(total)	NF(s-sp)	-	-	-	○	○
ASE FIT	GAUSS	-	-	-	○	○
SPECTRUM DIVISION	OFF	-	-	-	○	○
K Parameter(OPT AMP)	1	0.1	100	0.01	○	○
Masked SPAN(nm)	0.4	0	1100	0.01	○	○
Fitting SPAN(nm)	1	0	1100	0.01	○	○
FILTER $\Delta\lambda$ (nm)	0	0	1100	0.01	○	○
Pin LOSS(dB)	0	-10	10	0.01	○	○
Pout LOSS(dB)	0	-10	10	0.01	○	○
WDM LIST	OFF	-	-	-	×	×
WDM MODE	Multi Peak	-	-	-	○	○
WDM LIST ALL	OFF	-	-	-	○	○
WDM ASE Method	AUTO OFF	-	-	-	○	○
WDM THRESHOLD LVL (dB)	20	0.1	99.9	0.01	○	○
GRID Ref. Frequency (THz)	193.10	100	500	0.0001	○	○
GRID CH Spacing (GHz)	100.0	10	10000	0.1	○	○
Manual ASE Level (dBm)	-40	-90	23	0.01	○	○
ASE conversion NBW (nm)	1	0.01	10	0.001	○	○
ASE NBW Select	current	-	-	-	○	○
Reference CH No.	1	1	256	1	×	×
WDM Monitor	OFF	-	-	-	×	×
SPECTRUM display	OFF	-	-	-	○	○
GRAPH X	Time	-	-	-	○	○
DATA MODE	$\lambda.f$	-	-	-	○	○

## 3.4.1 Defaults Configuration Values

Table 3-2 Default Settings

Item	Default	Minimum value	Maximum value	Setting resolution	Backup	File save
ABSOLUTE/RELATIVE	ABS	-	-	-	○	○
Graph All Data	ON	-	-	-	○	○
Current Time No.	1	1	501	1	×	×
Current Channel No.	1	1	256	1	×	×
Measurement Times	11	1	501 Note 2	1	○	○
Time Interval (min.)	0.1	0.1	1440	0.1	○	○
Limit Judge Enable	disable	-	-	-	○	○
$\lambda$ Drift Limit (nm)	0.1	0.01	10	0.001	○	○
Nominal Level (dBm)	0	-90	+23	0.01	○	○
Level Upper Limit (dBm)	20	-90	+23	0.01	○	○
Level Lower Limit (dBm)	-20	-90	+23	0.01	○	○
Norminal SNR (dB)	20	0	60	0.01	○	○
SNR Lower Limit (dB)	10	0	60	0.01	○	○
DEVICE TYPE	Internal PRT	-	-	-	○	×
FLOPPY ON/OFF	OFF	-	-	-	○	×
FLOPPY FORMATTING	2HD	-	-	-	○	×
Bitmap Compless	OFF	-	-	-	○	×
Bitmap Save	Color	-	-	-	○	×
Color Pattern	PATTERN-1	-	-	1	○	×
Ext. PRT MODE	GRAY	-	-	-	○	×
Ext. PRT COMMAND	ESC/P	-	-	-	○	×
BUZZER(BEEP)	ON	-	-	-	○	×
WARNING	ON	-	-	-	○	×
QUIET BEEP	NORMAL	-	-	-	○	×

Note 2: When the analyzer is set to the monitoring function, up to 201 times if the number of WDM signals is between 65 and 128, or up to 101 times if the number of WDM signals is 129 or more.

Table 3-2 Default Settings

Item	Default	Minimum value	Maximum value	Setting resolution	Backup	File save
EXT Key	US	-	-	-	○	×
CLOCK ON/OFF	ON	-	-	-	○	×
MENU OUT(printer)	ON	-	-	-	○	×
CAL $\lambda$ (Int.)	-	-	-	-	○	×
CAL $\lambda$ (Ext.)	-	600	1700	0.001	○	×
$\lambda$ OFFSET(nm)	0	-100	100	0.001	○	○
LEVEL OFFSET(dB)	0	-20	20	0.01	○	○
RECALL OFFSET	OFF	-	-	-	○	×

○: The parameter is saved to Backup or File save.

×: The parameter is not saved to Backup or File save.

## 4 REMOTE CONTROL

### 4.1 GPIB Command Index

This GPIB command index can be used as the index for Chapter 4.

<u>GPIB Command</u>	<u>Pages</u>	<u>GPIB Command</u>	<u>Pages</u>
*IDN .....	4-40	FRQ.....	4-29
*TST .....	4-40	FSP.....	4-29
ALM.....	4-38	FTM.....	4-36
APC.....	4-29	GRF.....	4-34
ASP.....	4-32	GRI.....	4-32
AUL.....	4-32	GSP.....	4-34
AUT.....	4-30	HED(HD).....	4-38
AVG.....	4-30	IPR.....	4-38
AVS.....	4-30	LAB.....	4-31
BCP.....	4-37	LAR.....	4-35
BSV.....	4-37	LCC.....	4-35
BUZ.....	4-37	LCT.....	4-35
C(*RST).....	4-40	LDA.....	4-35
CEN.....	4-29	LEV.....	4-30
CKD.....	4-37	LFD.....	4-35
CLE.....	4-38	LHA.....	4-35
CLF.....	4-38	LIN.....	4-30
CLM.....	4-38	LLL.....	4-35
CLO.....	4-37	LMT.....	4-35
CLS.....	4-38	LNL.....	4-35
COP.....	4-37	LNS.....	4-35
CPT.....	4-37	LOS.....	4-33
CSB.....	4-38	LPF.....	4-39
CUC.....	4-29	LPI.....	4-34
CUD.....	4-31	LPO.....	4-34
CUL.....	4-30	LPR.....	4-33
CUR.....	4-31	LPS.....	4-31
DEL(DL).....	4-38	LPT.....	4-33
DEV.....	4-37	LRS.....	4-39
DLY.....	4-30	LSC.....	4-30
DMD.....	4-32	LSD.....	4-35
DUA.....	4-32	LSL.....	4-35
E(*TRG).....	4-39	LSP.....	4-29
EGE.....	4-30	LTF.....	4-35
EKB.....	4-37	LTI.....	4-35
EPM.....	4-37	LTM.....	4-35
FDL.....	4-34	LUL.....	4-35
FEE.....	4-37	LVA.....	4-35
FFO.....	4-37	MAL.....	4-36
FMT.....	4-38	MAT.....	4-32
FON.....	4-37	MCU.....	4-32

4.1 GPIB Command Index

MDA.....	4-32	QUI.....	4-37
MDC.....	4-32	RAU.....	4-30
MEA.....	4-31	RCL.....	4-33
MEN.....	4-37	REF.....	4-30
MMX.....	4-32	RES.....	4-30
MNC.....	4-30	RPS.....	4-31
MNH.....	4-30	S.....	4-38
MNT.....	4-32	SAV.....	4-32
MPT.....	4-32	SCR.....	4-34
MSK.....	4-38	SDL(DS).....	4-38
MSP(MS).....	4-38	SDV.....	4-34
MTE.....	4-32	SIM.....	4-32
MXC.....	4-30	SNA.....	4-36
MXH.....	4-30	SNB.....	4-36
NFK.....	4-34	SPA.....	4-29
NFT.....	4-34	SPT.....	4-32
NLV.....	4-33	SPW.....	4-33
NPK.....	4-34	SRQ.....	4-38
NWD.....	4-33	SRS.....	4-34
NWI.....	4-33	STA.....	4-29
OAM.....	4-34	STO.....	4-29
OCD.....	4-39	SWE.....	4-30
ODN.....	4-38	SYN.....	4-30
OGN.....	4-39	TRA.....	4-33
OLN.....	4-39	WAL.....	4-34
OLS.....	4-39	WAR.....	4-37
OLT.....	4-39	WAU.....	4-36
OMD.....	4-34	WDM.....	4-34
ONT.....	4-39	WMD.....	4-34
ONW.....	4-39	WPK.....	4-33
OPA.....	4-39	WPR.....	4-33
OPK.....	4-38	WPW.....	4-33
OPM.....	4-39	WPX.....	4-33
OPN.....	4-39	WPY.....	4-33
OSD.....	4-38	WRF.....	4-34
OSW.....	4-39	WTY.....	4-33
OVS.....	4-38	WYD.....	4-36
OWN.....	4-39	XAC.....	4-31
OWP.....	4-39	XAS.....	4-31
PAN.....	4-39	XBC.....	4-31
PAS.....	4-39	XBS.....	4-31
PGT.....	4-30	XUL.....	4-32
PIN.....	4-33	YAC.....	4-31
PKC.....	4-29	YAS.....	4-31
PKL.....	4-30	YBC.....	4-31
PLV.....	4-34	YBS.....	4-31
PLW.....	4-34		
PMO.....	4-33		
PNR.....	4-33		
PNX.....	4-33		
PRT.....	4-37		

## 4.2 Overview of GPIB

The GPIB is an interface connected to the measurement device, controller, and peripheral units, etc., through a simple cable (bus line).

The GPIB is more expandable than conventional interfaces, is easy to use, and has electrical, mechanical, and functional compatibility with other manufacturers' products, making it applicable to system configurations from simple systems to automatic design systems with high-level functions using one bus cable.

To use the GPIB, first setting an "address" for each instrument connected to the bus line is required. Each instrument is assigned one or more roles from the following three roles: controller, talker (TALKER), or listener (LISTENER).

During system operation, only one "talker" can send data to the bus line, but plural "listeners" can receive it.

The controller specifies the addresses of "talker" and "listener" to transfer data from "talker" to "listener", and the controller sets setting conditions from "talker" to "listener".

Data is synchronously transferred synchronously bidirectionally between devices via eight data lines in the bit-parallel, byte-serial form. Because this is a synchronous system, using high-speed and low-speed devices together in the same system is possible.

Data (messages) transferred between devices include measurement data, measurement conditions (programs), and commands; they are in ASCII.

In addition to eight data lines, the GPIB has three handshake lines for controlling the synchronous data transmission between instruments, and five control lines for controlling the bus information flow.

## 4.3 Interface Functions

**4.3 Interface Functions**

Table 4-1 shows analyzer interface functions.

**Table 4-1 Interface Functions**


Code	Function
SH1	Source handshake
AH1	Acceptor handshake
T6	Basic talker Serial polling Talker reset based on listener specification
L4	Basic listener Listener reset based on talker specification
SR1	Service request
RL1	Remote
PP0	No parallel function
DC1	Device clear
DT1	Device trigger
C0	No controller function
E2	Three-state-bus-driver used



## 4.4 Program Code

This section explains the program code through which the outside controller sets analyzer conditions.

Each program code consists of three English characters which indicate the functions and numerical data for setting functions as follows:

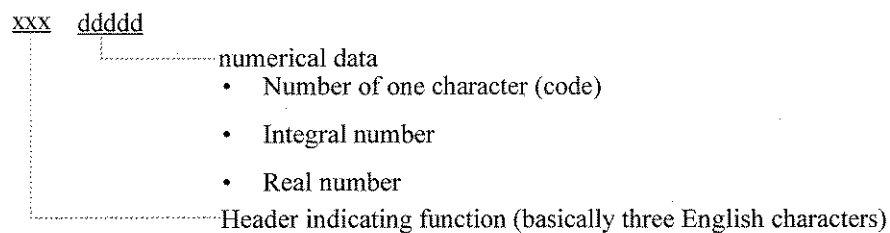

The state of each condition is read in by adding “?” after the functional header.

---

**NOTE:**

1. *For the functional header and unit, either a capital letter or a lower-case letter is used for setting. Any space code (20H) is set in a program code.*
  2. *In this analyzer, the program code is processed in one row to the terminator. The maximum allowable characters set in one row are 255.  
When describing a plurality of program codes in one row, set the program codes by punctuating with comma (,) or semicolon (;).*
-


4.5 Talker Formats (Data Output Formats)

4.5 Talker Formats (Data Output Formats)

This section describes the talker formats used when this analyzer system transfers data to an external controller.

Data is classified roughly into eleven types of formats.

- (1) Waveform data (program code "OSD0", "OSD1", "OSD2", "OSD3", "OPA")
  - ASCII format (format specification code "FMT0")

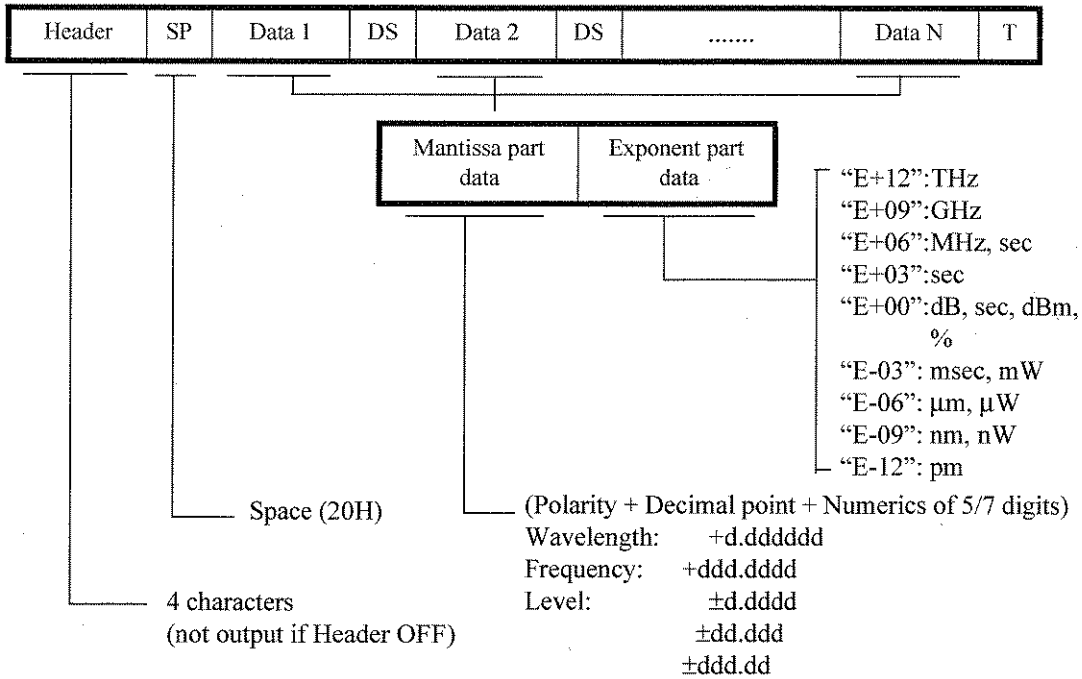

Header	Data type
LMUM	Wavelength [m]
FQTH	Frequency [Hz]
LVLG	Level data in logarithmic scale [dB, dBm]
LVLI	Level data in linear scale
LVPC	Level data of unit %
TM S	Time data in trend chart
OPA	ASE fitting data [dBm]

- DS: Data Separator (either ',' or ';' CR or NL)  
Can be specified by the program code "SDLn" ("DSn").
- T: Terminator (either NL<EOI>, NL<EOI> or "CR,NL<EOI>")  
Can be specified by the program code "DELn" ("DLn").


- BINARY format (format specification code (“FMT1”, “FMT2”, “FMT3”, “FMT4”))



Is output in either of the following four formats according to the setting of the format specification code “FMTn.”


- (a) “FMT1” ... 16 bits (integer type)

Is output within the range of 0 to 10000 on the X axis and within 0 to 10000 on the Y axis by setting all data on the screen as linear scale.

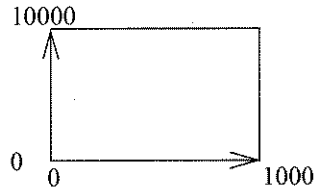

- (b) “FMT2” ... 64 bits (floating point type)

Outputs data in the floating-point format (IEEE Std.754-1985 format) as shown below.

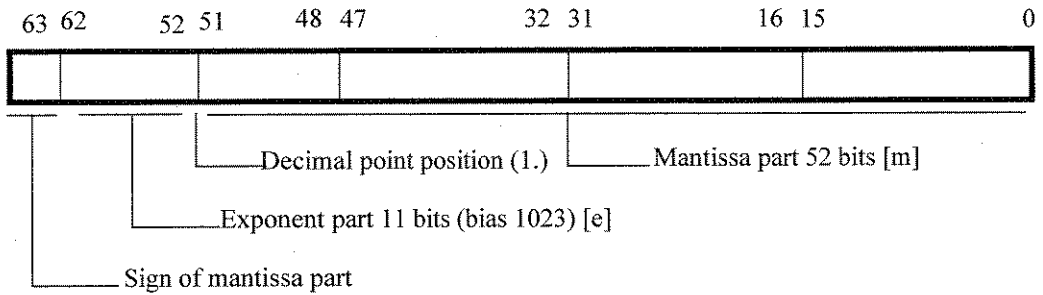


The formula is shown below.

$$(-1)^S \times 1.m \times 2^{(e-1023)}$$

4.5 Talker Formats (Data Output Formats)

(c) "FMT3" ... 32 bits (IEEE floating-point type)

Outputs data in the floating-point format (IEEE Std.754-1985 format) as shown below.

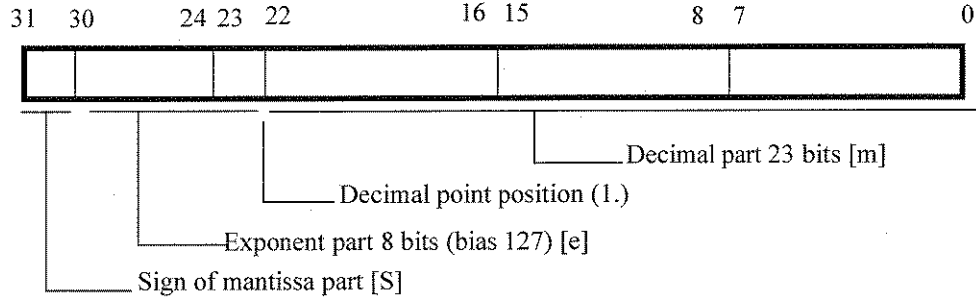


The formula is shown below.

$$(-1)^S \times 2^{(e-127)} \times 1.m$$

(d) "FMT4" ... 32 bits (NEC floating point type)


Outputs data in the floating-point format (NEC-PC internal format) shown below.

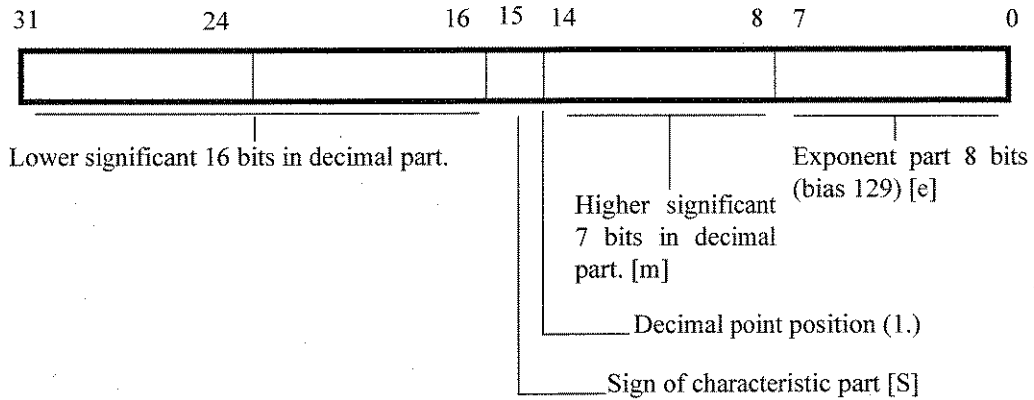

The formula is expressed below.

$$(-1)^S \times 1.m \times 2^{(e-1023)}$$


- (2) Peak search data (Program code "OPK")
  - Spectrum measurement

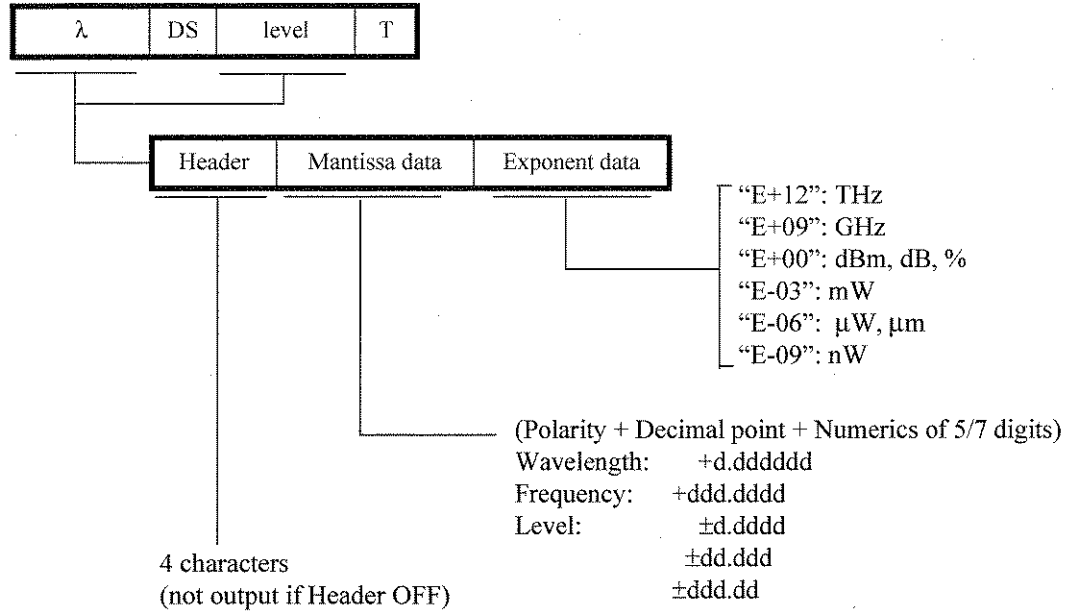

Header	Data type
LMPK	Peak wavelength ( $\lambda$ )
LQPK	Peak frequency (f)
LVPK	Peak level (level)

4.5 Talker Formats (Data Output Formats)

- Power monitor display

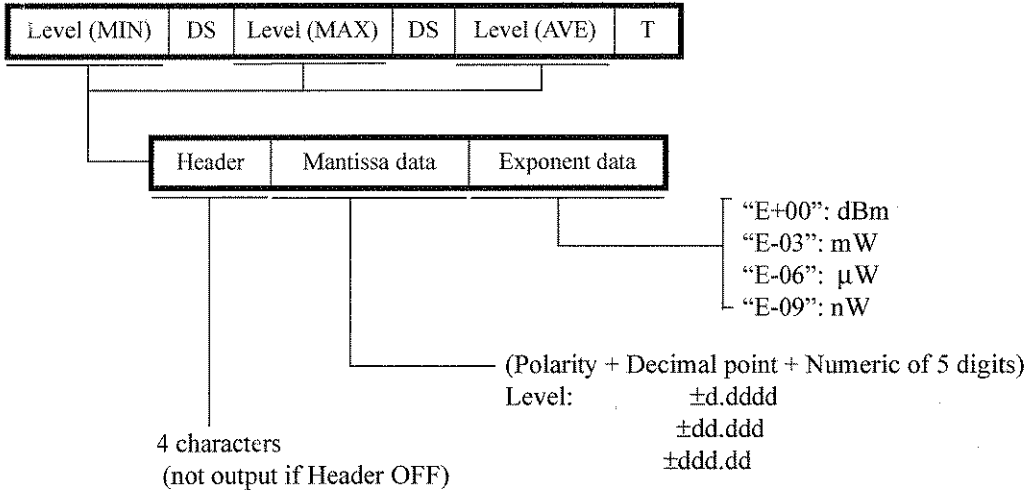


Header	Data type
LVMN	Minimum of the level data
LVMX	Maximum of the level data
LVAV	Average value of the level data

(3) Cursor data (Program code "OCD")

One of the following four formats is used according to the "CUDn" code for specifying the cursor display mode.

(In power monitor display, the cursor data output is fixed not according to the "CUDn".)

- "CUD0" ... Normal

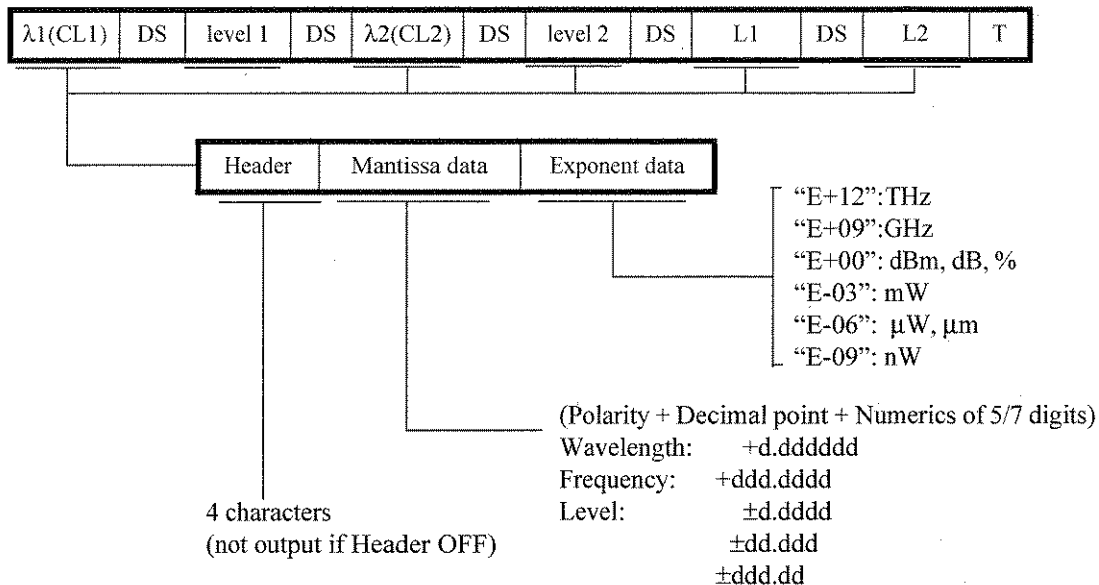

Header	Data type
LMXA	Wavelength of X cursor 1 ( $\lambda_1$ )
FQXA	Frequency of X cursor 1 (f1)
LVXA	Level of X cursor 1 (level 1)
LMXB	Wavelength of X cursor 2 ( $\lambda_2$ )
FQXB	Frequency of X cursor 2 (f2)
LVXB	Level of X cursor 2 (level 2)
LVYA	Level of Y cursor 1 (L1)
LVYB	Level of Y cursor 2 (L2)

DS: Data Separator (“,” , “;”, CR or NL)

Can be specified with program code “SDLn” (“DSn”).

T: Terminator (NL<EOI>, NL, <EOI>, or CR, NL<EOI>)

Can be specified using program code “DELn” (“DLn”).

**NOTE:** The mantissa and exponent formats are common to all “CUDn” codes.

4.5 Talker Formats (Data Output Formats)

- “CUD0” ... Normal(Case of minimum/maximum hold mode)

$\lambda 1$	DS	level1	DS	level2	DS	level3	DS	$\lambda 2$	DS	level4	DS	level5	DS	level6	T
-------------	----	--------	----	--------	----	--------	----	-------------	----	--------	----	--------	----	--------	---

Header	Data type
LMXA	Wavelength of X cursor 1 ( $\lambda 1$ )
FQXA	Frequency of X cursor 1 (f1)
MXXA	Maximum hold level of X cursor 1 (level 1)
LVXA	Current waveform level of X cursor 1 (level 2)
MNXA	Minimum hold level of X cursor 1 (level 3)
LMXB	Wavelength of X cursor 2 ( $\lambda 2$ )
FQXB	Frequency of X cursor 2 (f2)
MXXB	Maximum hold level of X cursor 2 (level 4)
LVXB	Current waveform level of X cursor 2 (level 5)
MNXB	Minimum hold level of X cursor 2 (level 6)

- “CUDI” ...  $\Delta$ MODE

$\lambda 1$	DS	level 1	DS	$\Delta \lambda$	DS	$\Delta$ level	DS	L1	DS	$\Delta L$	T
-------------	----	---------	----	------------------	----	----------------	----	----	----	------------	---

Header	Data type
LMXA	Wavelength of X cursor 1 ( $\lambda 1$ )
FQXA	Frequency of X cursor 1 (f1)
LVXA	Level of X cursor 1 (level 1)
LMDX	Wavelength difference between X cursor 1 and 2 ( $\Delta \lambda$ )
FQDA	Frequency difference between X cursor 1 and 2 ( $\Delta f$ )
LVDX	Level difference between X cursor 1 and 2 ( $\Delta$ level)
LVYA	Level of X cursor 1 (L1)
LVDY	Level difference between Y cursor 1 and 2 ( $\Delta L$ )



- “CUD1” ... ΔMODE (Case of minimum/maximum hold mode)

$\lambda 1$	DS	level1	DS	level2	DS	level3	DS	$\lambda 2$	DS	level4	DS	level5	DS	level6	T
-------------	----	--------	----	--------	----	--------	----	-------------	----	--------	----	--------	----	--------	---

Header	Data type
LMXA	Wavelength of X cursor 1 ( $\lambda 1$ )
FQXA	Frequency of X cursor 1 (f1)
MXXA	Level difference between max hold and min hold at X cursor 1 (level 1)
MCXA	Level difference between max hold and Current at X cursor 1 (level 2)
CMXA	Level difference between Current and min hold at X cursor 1 (level 3)
LMXB	Wavelength of X cursor 2 ( $\lambda 2$ )
FQXB	Frequency of X cursor 2 (f2)
MMXB	Level difference between max hold and min hold at X cursor 2 (level 4)
MCXB	Level difference between max hold and Current at X cursor 2 (level 5)
CMXB	Level difference between Current and min hold at X cursor 2 (level 6)

- “CUD2” ... 2ND PEAK

$\lambda 1$	DS	level 1	DS	$\Delta\lambda$	DS	$\Delta\text{level}$	T
-------------	----	---------	----	-----------------	----	----------------------	---

Header	Data type
LMPK	Peak wavelength ( $\lambda 1$ )
FQPK	Peak frequency (f1)
LVPK	Peak level (level 1)
LMDP	Wavelength difference between 1st and 2nd peaks ( $\Delta\lambda$ )
FQDP	Frequency difference between the 1st and the 2nd peaks ( $\Delta f$ )
LVDP	Level difference between 1st and 2nd peaks ( $\Delta\text{level}$ )

4.5 Talker Formats (Data Output Formats)

- “CUD3” ... POWER

$\lambda 1$	DS	$\lambda 2$	DS	$\Sigma L$	T
-------------	----	-------------	----	------------	---

Header	Data type
LMXA	Wavelength of X cursor 1 ( $\lambda 1$ )
FQXA	Frequency of X cursor 1 (f1)
LMXB	Wavelength of X cursor 2 ( $\lambda 2$ )
FQXB	Frequency of X cursor 2 (f2)
LVPW	Sum of levels between X cursor 1 and 2 ( $\Sigma L$ ).

- “CUD4” ... Peak to Peak

$\lambda 1$	DS	level 1	DS	$\lambda 2$	DS	level 2	DS	$\Delta \lambda$	DS	$\Delta level$	T
-------------	----	---------	----	-------------	----	---------	----	------------------	----	----------------	---

Header	Data type
LMXA	Wavelength of X cursor 1 ( $\lambda 1$ ).
FQXA	Frequency of X cursor 1 (f1).
LVXA	Level of X cursor 1 (level 1).
LMXB	Wavelength of X cursor ( $\lambda 2$ ).
FQXB	Frequency of X cursor 2 (f2).
LVXB	Level of X cursor 2 (level 2).
LMPP	Wavelength difference of maximum and minimum ( $\Delta \lambda$ ).
FQPP	Frequency difference between the maximum and the minimum values ( $\Delta f$ ).
LVPP	Level difference of Maximum and minimum ( $\Delta level$ ).

- Cursor data output in power monitor display (trend chart)

No	DS	level	T
----	----	-------	---

(Integer of 4 digits)  
dddd


The exponent part and mantissa part are the same  
as the usual level data.

Header	Data type
NOTC	Data number at cursor position.
LVTC	Level data at cursor position.

4.5 Talker Formats (Data Output Formats)

- (4) Spectral width data and notch width data (Program code “OSW”, “ONW”)

The results of four types of calculations are all output in the following format:

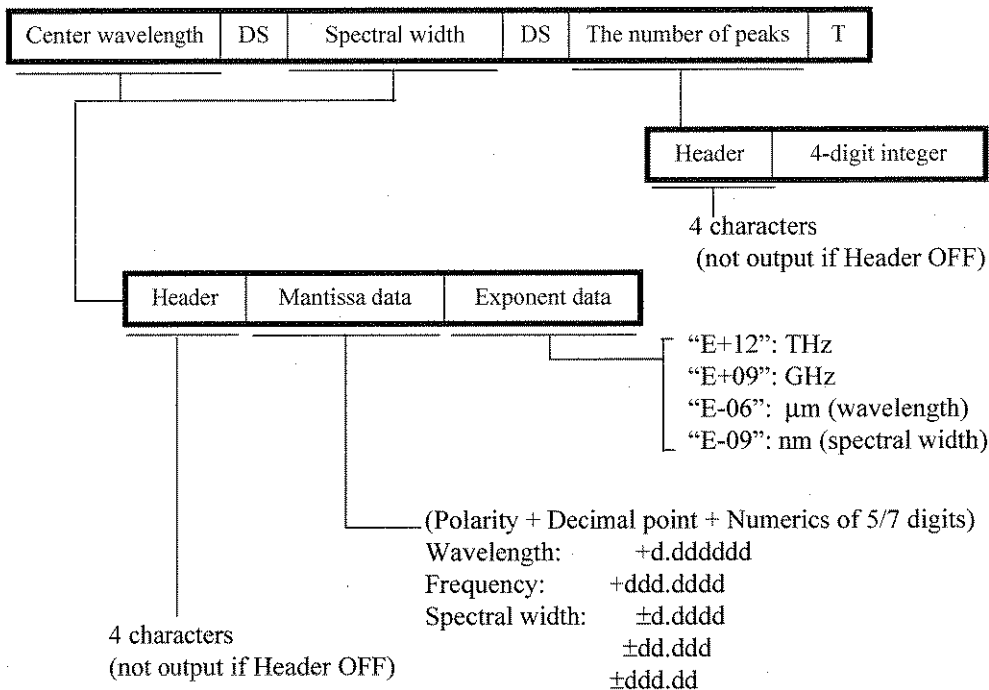


Header	Data type
LMCN	Center wavelength
FQCN	Center frequency
LMHW	Spectral wavelength width
FQHW	Spectral frequency width
NOSP	Numbers of peaks

DS: Data Separator (“,” “;”, CR or NL)  
Can be specified with program code “SDLn” (“DSn”).

T: Terminator (NL<EOI>, NL, <EOI> or CR, NL<EOI>)  
Can be specified using program code “DELn” (“DLn”).


(5) GPIB output format of gain and noise figure operation result (“OGN”).

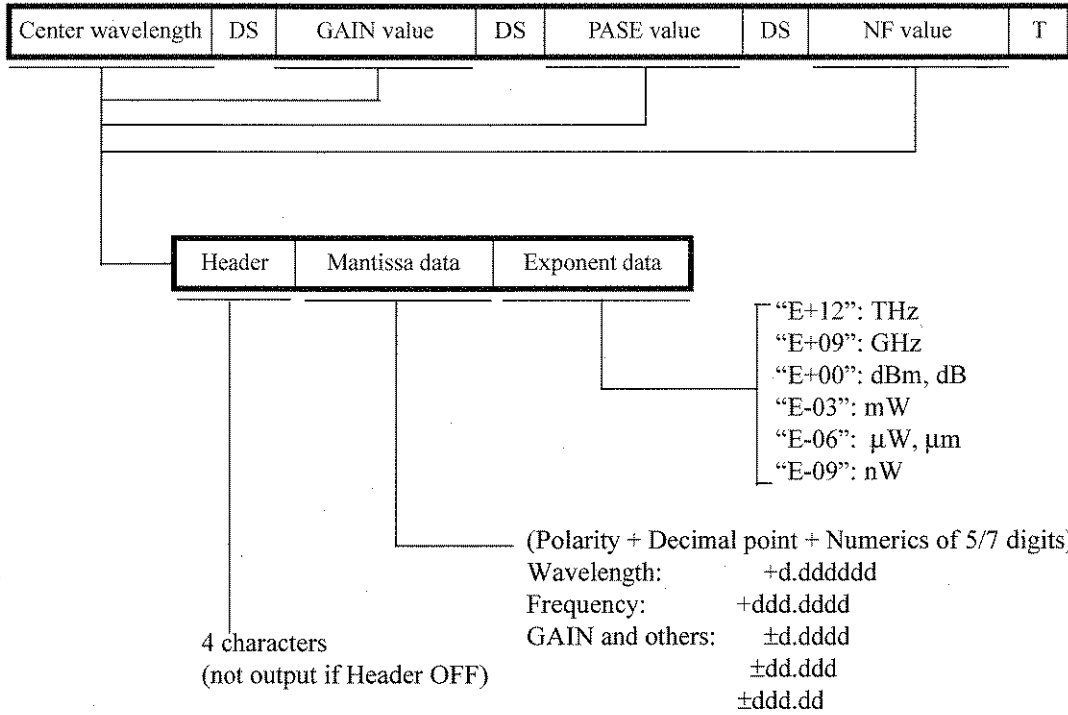

Header	Data type
LMCN	Center wavelength
FQCN	Center frequency
GAIN	GAIN value
PASE	PASE value
NF	NF value

4.5 Talker Formats (Data Output Formats)

(6) GPIB output format of gain, noise figure and total ASE power operation result (“OPN”).

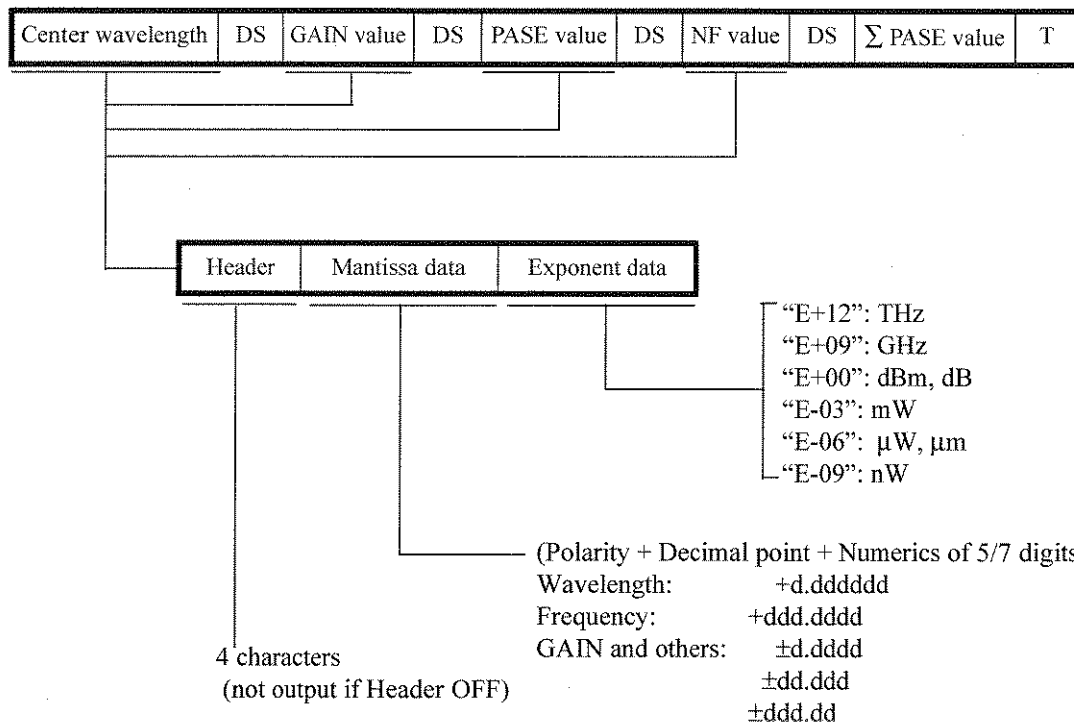

Header	Data type
LMCN	Center wavelength
FOCN	Center frequency
GAIN	GAIN value
PASE	PASE value
NF	NF value
PSPW	ΣPASE value (Total ASE power)

(7) List data output (“OLS”)


- OPE, AMP and WDM operation results 1

Operation results are output for the number of peaks (the value read by OWP) of the output formats shown in (5) “OGN”. However, the terminator is sent at the last of the output only. The terminator is sent only to the end of the output.

- Multi peak

Operation results are output for the number of peaks (the value read by OLN) of the output formats shown in (2) “OPK”. However, the terminator is sent at the last of the output only. The terminator is sent only to the end of the output.


- SNR

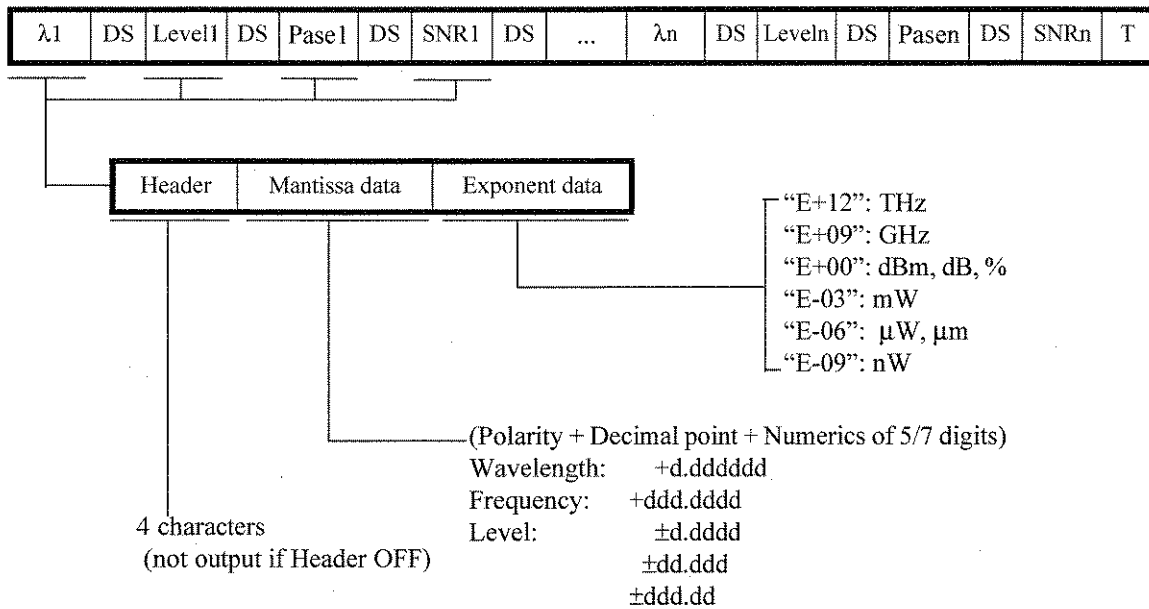

Header	Data type
LMLS	Wavelength
FQLS	Frequency
LVLS	Level value
PASE	PASE value
SNR	SNR value

4.5 Talker Formats (Data Output Formats)

- Relative



- “E+12”: THz
- “E+09”: GHz
- “E+00”: dBm, dB, %
- “E-03”: mW
- “E-06”: μW, μm
- “E-09”: nW

(Polarity + Decimal point + Numerics of 5/7 digits)

Wavelength: +d.ddddd

Frequency: +ddd.dddd

Level: ±d.dddd

±dd.ddd

±ddd.dd



4 characters

(not output if Header OFF)

Header	Data type
LMLS	Wavelength
FQLS	Frequency
LSPC	Spacing value (wavelength)
FSPC	Spacing value (frequency)
LMRF	λ-Ref value (wavelength)
FMRF	f-Ref value (frequency)
LVLS	Level value
LVRF	L-Ref value



• ITU-GRID

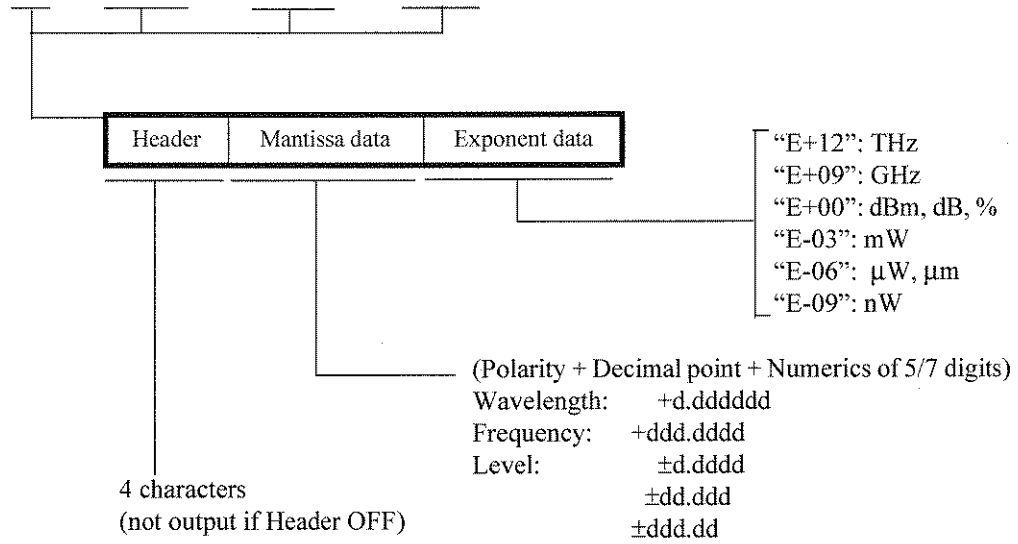



Header	Data type
LMLS	Wavelength
FQLS	Frequency
LMGD	GRID wavelength
FQGD	GRID frequency
LMRG	$\lambda$ -GRID value (wavelength)
FQRG	f-GRID value (frequency)
LVLS	Level value

4.5 Talker Formats (Data Output Formats)

(8) GPIB output format of Opt.AMP result 2 (“OWN”)

This format has the level values of all signals added to the “OGN” output format described in paragraph (5).

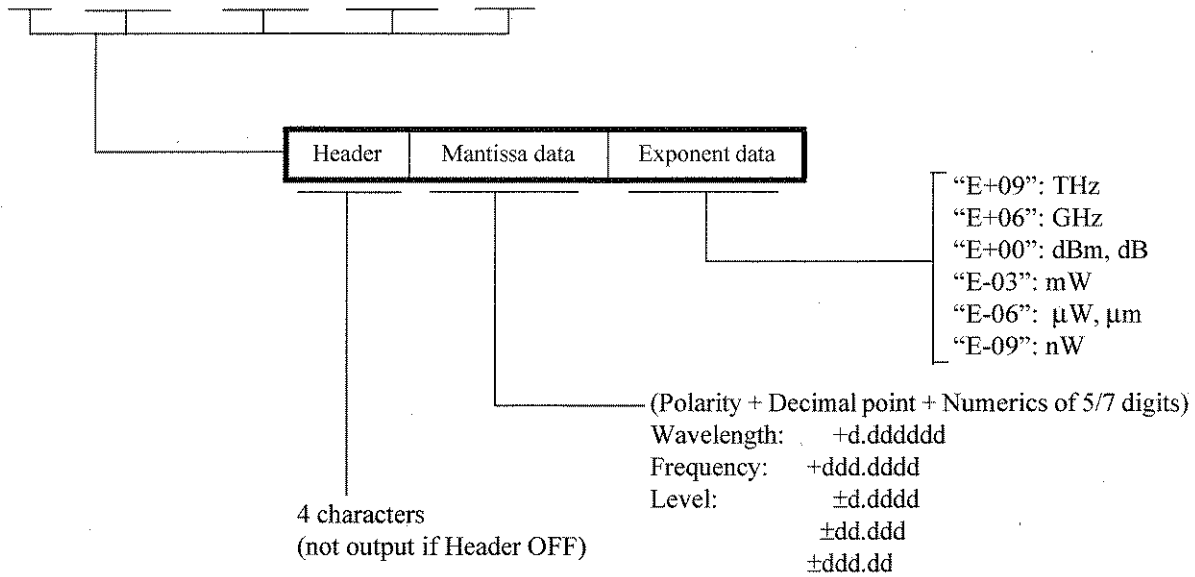


Header	Data type
LMCN	Center wavelength
FQCN	Center frequency
POUT	Level value
GAIN	GAIN value
PASE	PASE value
NF	NF value

(9) GPIB output format used in the WDM monitor data table (OLTxxx)

- When Pass/Fail is set to OFF

Outputs the measurement time number and the nth measurement data.


The data group consisting of  $\lambda$ , level and SNR is output once for each peak (that has been loaded using OLS)

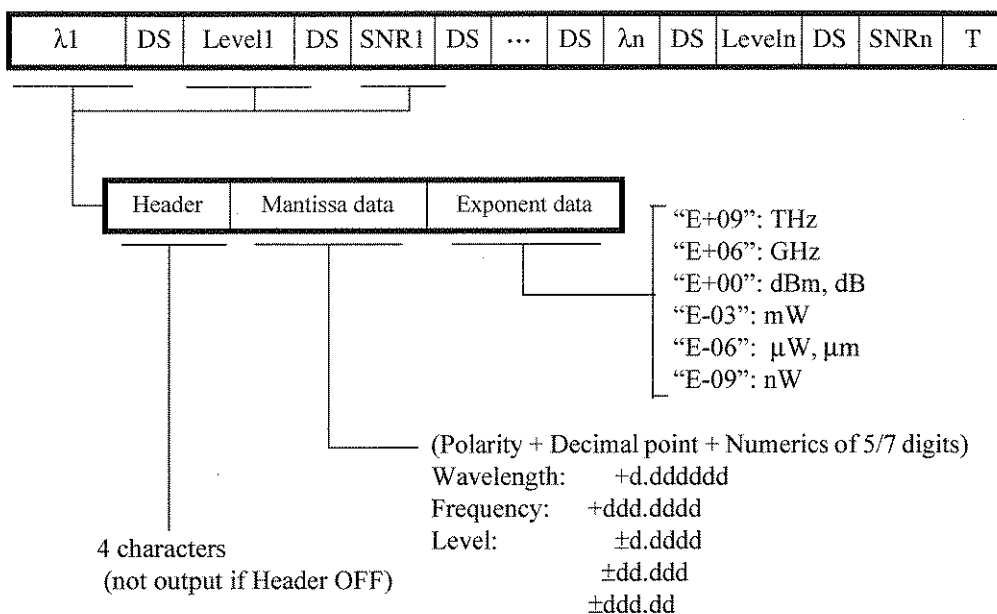

Header	Data type
LMLS	Wavelength
FQLS	Frequency
LVLS	Level value
SNR	SNR value

4.5 Talker Formats (Data Output Formats)


- When Pass/Fail is set to ON  
A data group consisting of  $\lambda$ , level and SNR, and the Pass/Fail judgment for each parameter are output once for each peak (that has been loaded using OLS).

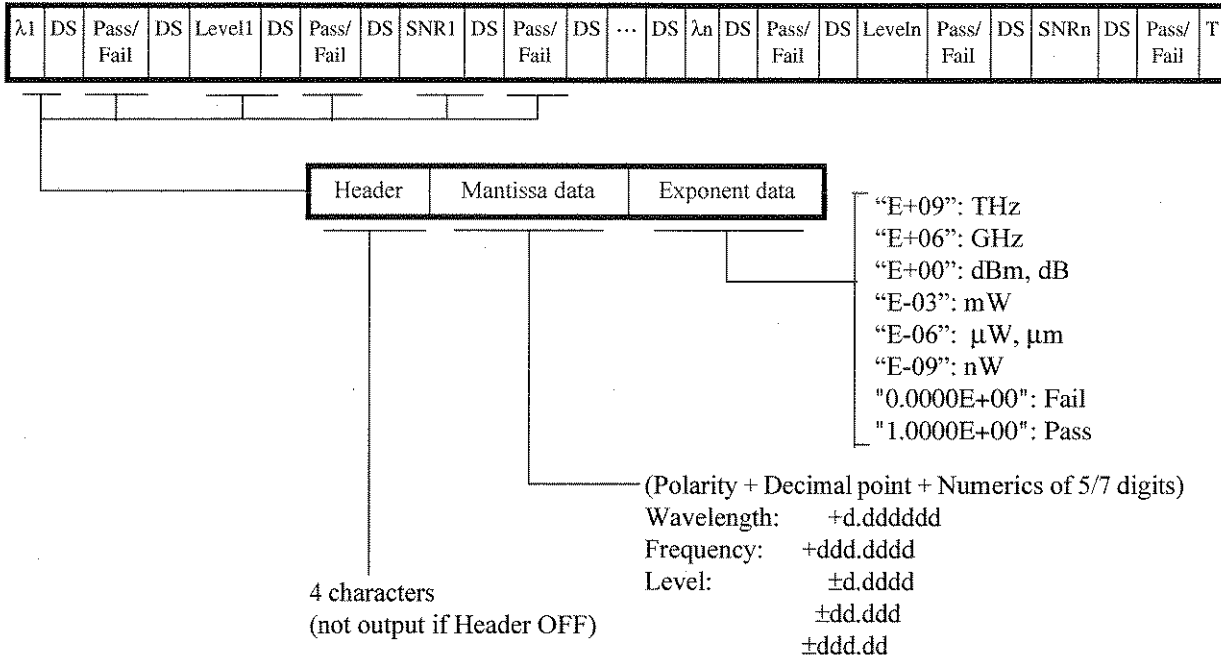

Header	Data type
LMLS	Wavelength
FQLS	Frequency
LVLS	Level value
SNR	SNR value
PSLM	Pass/Fail for the wavelength (frequency)
PSLV	Pass/Fail for the level
PSSR	Pass/Fail for SNR

(10) Device identification

When program code “\*IDN?” is received, the following data is output:

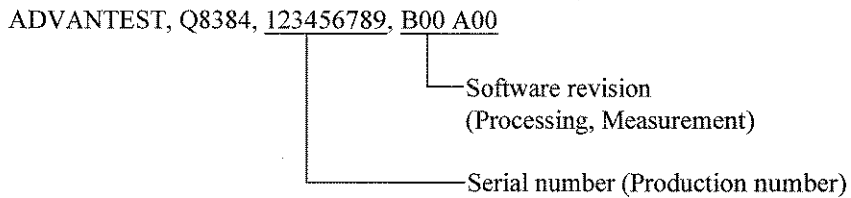

## (11) Setting condition data

The current setting state can be read by using “?” instead of setting data if the code is readable.

The setting state is output in the following format:

Header	Data	T
--------	------	---

- 1-digit integer (unsigned)  
APC, RAU, LIN, LEV, SWE, CUR, XAC, XBC, YAC, YBC, CUD, MEA, DUA, SIM, GRI, AUL, PNR, LOS, TRA, SPW, WTY, PMO, OAM, NFT, FTM, SDV, NPK, WDM, WAU, DEV, FON, BUZ, WAR, QUI, CKD, MEN, SRQ, HED, DEL, SDL, MSP, FMT, OVS, MNH, MXH, AUT, AVM, SYN, EGE, NWD, OMD, WMD, EPM, CPT, BSV, BCP, FFO, PRT, OSD, SPT, SNE, FRQ, ASP, MTE, NPK, SRS, WAL, LTM, LSD, LHA, LVA, LAR, LDA, LTF, EKB
  - 2-digit integer (unsigned)  
AVG, SMN, AVS, MMX, MCU
  - 3-digit integer (unsigned)  
MSK, LMT, LCT, LCC, WRF
  - 4-digit integer (unsigned)  
PNX
  - Mantissa data + Exponent data
    - “E+00”: dBm, dB, %
    - “E-03”: mW, mm
    - “E-06”:  $\mu$ W,  $\mu$ m
    - “E-09”: nW

(Polarity + Decimal point + Numerics of 5/6 digits)  
Wavelength: +d.ddddd  
Level:  $\pm$ d.dddd  
(Time)  $\pm$ dd.ddd  
 $\pm$ ddd.dd
- Note: The polarity at time is only +.
- CEN, SPA, STA, STO, REF, PGT, XAS, XBS, YAS, YBS, WPX, WPY, WPK, WPR, PIN, NFK, SNA, SNB, FDL, LPI, LPO, PLV, PLW, WYD, RES, DLY, NLV, NWI, CLE, WPW, CLF, CLS, LTI, LSC, GRF, GSP, SCR, LFD, LNL, LLL, LNS, LSL, MAL
- Others  
LAB: 1 to 48 characters  
CLO: YY-MM-DD, hh:mm:ss  
SAV, DMD, RCL: 1 to 11 characters

Same as the functional header specified.

## 4.6 Device Triggering Function

## 4.6 Device Triggering Function

This analyzer system performs a SINGLE measurement operation similar to the case in which it receives the program codes "MEAL," "E" and "\*TRG" through the address specification command 'GET' (Group Execute Trigger).

## 4.7 Device Clear Function

This analyzer system is set to the initial state when turning the power on, similar to the case in which it receives the program codes "C" and "\*RST" through the address specification command 'SDC' (Selected Device Clear) and the universal command 'DCL' (Device Clear).

The initial state after turning the power on is shown in Table 4-2.

Table 4-2 Initial State After Turning the Power On

Item	Initial state
1. Measurement conditions (FUNCTION section)	Previous state
2. Data display	Normal display (Dual screen, superimposing and list display are all OFF).
3. Cursor display	All are OFF.
4. Half width calculation	OFF
5. GPIB-related Status byte Masking status bytes Transmission of SRQ signal Output format of waveform data Terminator Data separator	0 (Clear) "MSK0" (No mask) "SRQ0" (Mode in which the SQR signal is not sent) "FMT0" (ASCII) "DEL0" (DL0) ⇒(NL<EOI>) "SDL0" (DS0) ⇒(,)

## 4.8 State Changes According to the Commands

This analyzer system will be in the states listed in Table 4-3 after turning the power on and receiving the various commands.

**Table 4-3 State Changes According to the Commands**

Command code	Talker	Listener	Remote	SRQ	Status byte	Transferred data	Parameters and Operation State
POWER ON	Clear	Clear	Local	Clear	Clear	Clear	Partial initialization
IFC	Clear	Clear	-	-	-	-	-
DCL	-	-	-	Clear	Clear	Clear	Partial initialization
SDC	Clear	Set	-	Clear	Clear	Clear	Partial initialization
C, *RST	Clear	Set	Remote	Clear	Clear	Clear	Partial initialization
IPR	Clear	Set	Remote	Clear	Clear	Clear	Initialization
GET	Clear	Set	-	=	Clear b0, 2, 3 and 5	Clear	-
E, *TRG	Clear	Set	Remote	=	Clear b0, 2, 3 and 5	Clear	-
Specifying the talker for this analyzer system.	Set	Clear	-	-	-	-	-
Command for turning the talker off.	Clear	-	-	-	-	-	-
Specifying the listener for this analyzer system.	Clear	Set	-	-	-	-	-
Command for turning the listener off.	-	Clear	-	-	-	-	-
Serial polling	Set	Clear	-	Clear	-	-	-

-: Indicates that the previous state does not change.

=: Indicates indefinite state

DCL: Device Clear

SDC: Selected Device Clear

GET: Group Execute Trigger

4.9 Status Byte

**4.9 Status Byte**

The functions of each bit in the status byte (used for this analyzer system) are shown below.

b7	b6	b5	b4	b3	b2	b1	b0
----	----	----	----	----	----	----	----

- b0: measure end  
Set to 1 at the end of calibration and alignment.  
Set to 0 upon starting the next measurement.
- b1: syntax error  
Set to 1 if there are any grammatical/setting errors in the received program codes.  
Set to 0 upon receiving the next program codes.
- b2: calculation end  
Set to 1 at the end of half width calculation.  
Set to 0 upon starting a measurement.
- b3: copy end or floppy access end  
Set to 1 at the end of printer output or access to the floppy disk (writing, reading or initialization).  
Set to 0 upon starting a measurement, receiving an "COP" code.
- b4: trend end  
Set to 1 when one trend chart measurement is completed on the power monitor display.  
Set to 0 when the next trend measurement is started.
- b6: RQS  
Is the bit that indicates that it is issuing a service request and Set to 1 if any of bits b0 to b5 and b7 is 1.  
Set to 0 if all bits are 0.
- b7: self-test error  
Set to 1 if any abnormality occurs while performing the self-test function.  
Set to 1 when a calibration or alignment is abnormally terminated.



## 4.10 GPIB Command Codes

The following tables list the GPIB commands by function.

- Listener Code Column: An asterisk (\*) in the Listener Code Column indicates that the function requires numeric data together with the function code.

Table 4-4 FUNCTION (1 of 2)

Function		Header	Query	Contents
CENTER	CENTER	CEN *	CEN?	Unit When the horizontal axis is set to wavelength UM: $\mu\text{m}$ (default setting), NM: nm When the horizontal axis is set to frequency THZ: THz(default setting), GHZ: GHz
	PEAK	PKC	-	peak to center
	CURSOR	CUC	-	cursor to center
	AUTO PKC	APC *	APC?	Auto Peak Center 0:OFF, 1:ON
SPAN	SPAN	SPA *	SPA?	Unit When the horizontal axis is set to wavelength UM: $\mu\text{m}$ (default setting), NMD: nm/DIV When the horizontal axis is set to frequency THZ: THz(default setting), GHZ: GHz THZD:THz/DIV, GHZD:GHz/DIV Example: SPA12.3NM
	START	STA *	STA?	Unit When the horizontal axis is set to wavelength UM: $\mu\text{m}$ (default setting), NM: nm When the horizontal axis is set to frequency THZ: THz(default setting), GHZ: GHz
	STOP	STO *	STO?	Unit When the horizontal axis is set to wavelength UM: $\mu\text{m}$ (default setting), NM: nm When the horizontal axis is set to frequency THZ: THz(default setting), GHZ: GHz
	Cursor SPAN	LSP	-	$\lambda_1 \leftrightarrow \lambda_2$ set to span
	FULL	FSP	-	FULL SPAN 0.6 to 1.70 $\mu\text{m}$ (setting wavelength 176.349 to 499.654 THz)
	Wavelength/Frequency	FRQ *	FRQ?	Setting the horizontal axis 0: Wavelength, 1: Frequency

4.10 GPIB Command Codes

Table 4-4 FUNCTION (2 of 2)

Function		Header	Query	Contents
REF LEVEL	REF LEVEL	REF *	REF?	Unit DBM: dBm(default setting), MW: mW, UW: $\mu$ W, NW: nW
	PEAK	PKL	-	ref-level set to peak
	CURSOR	CUL	-	ref-level set to cursor
	MAX HOLD→CURRENT	MXC	-	Specifying the waveform in MAX HOLD for the current waveform.
	MIN HOLD→CURRENT	MNC	-	Specifying the waveform in MIN HOLD for the current waveform.
	MAX HOLD	MXH *	MXH?	0: OFF, 1: ON
	MIN HOLD	MNH *	MNH?	0: OFF, 1: ON
	AUTO	RAU *	RAU?	0: OFF, 1: ON
LEVEL SCALE	LEVEL SCALE	LEV *	LEV?	-1: other, 0: 10dB/D, 1: 5dB/D, 2: 2dB/V, 3: 1dB/D, 4: 0.5dB/D, 5: 0.2dB/D, 6: 0.1dB/D
		LSC *	LSC?	Setting range: 0.1 to 10
	LIN/LOG	LIN *	LIN?	0: LOG, 1: LINEAR
AUTO	AUTO	AUT *	-	0: ABORT(STOP), 1, 2, 3: START
AVERAGE	POINT AVERAGE	AVG *	AVG?	Setting range: 1(OFF) to 64
	SWEEP AVERAGE	AVS *	AVS?	Setting range: 1(OFF) to 64
	SMOOTHING	SMN *	SMN?	Setting range: 1(OFF), 3, 5, 7, 9, 11
SWEEP MODE	SWEEP MODE	SWE *	SWE?	0: NORMAL, 1: ADAPTIVE, 2: HI-SENS1, 3: HI-SENS2, 4: PULSE, 5: HI-DYNAMIC1, 6: HI-DYNAMIC2
	GateTime	PGT *	PGT?	Unit SEC: sec(default setting), MSEC: msec
	SYNC	SYN *	SYN?	0: LOW, 1: HI
	DELAY	DLY *	DLY?	Sync HI Delay Time[ $\mu$ sec], 0 to 1000
	EDGE	EGE *	EGE?	0: RISE, 1: FALL
RESOLUTION		RES *	RES?	Unit UM; $\mu$ m, NM:nm(default setting)

Table 4-5 CURSOR

Function		Header	Query	Contents
CURSOR ON/OFF		CUR *	CUR?	0: CURSOR OFF, 1: CURSOR ON
$\lambda 1$	ON/OFF	XAC *	XAC?	0: $\lambda 1$ OFF, 1: $\lambda 1$ ON
	SET $\lambda 1$	XAS *	XAS?	When the horizontal axis is set to the wavelength: UM: $\mu\text{m}$ (Default), NM: nm When the horizontal axis is set to frequency: THZ: THz (Default), GHz:GHz
$\lambda 2$	ON/OFF	XBC *	XBC?	0: $\lambda 2$ OFF, 1: $\lambda 2$ ON
	SET $\lambda 2$	XBS *	XBS?	When the horizontal axis is set to the wavelength: UM: $\mu\text{m}$ (Default), NM: nm When the horizontal axis is set to frequency: THZ: THz (Default), GHz:GHz
L1	ON/OFF	YAC *	YAC?	0: L1 OFF, 1: L1 ON
	SET L1	YAS *	YAS?	Unit DBM: dBm, DB: dB, MW: mW, UW: $\mu\text{W}$ , NW: nW, PC: %
L2	ON/OFF	YBC *	YBC?	0: L2 OFF, 1: L2 ON
	SET L2	YBS *	YBS?	Unit DBM: dBm, DB: dB, MW: mW, UW: $\mu\text{W}$ , NW: nW, PC: %
CURSOR DATA		CUD *	CUD?	0: NORMAL, 1: $\Delta$ MODE, 2: 2nd PEAK, 3: POWER, 4: PEAK TO PEAK
LEFT PEAK		LPS	-	$\lambda 1$ set next left peak
RIGHT PEAK		RPS	-	$\lambda 1$ set next right peak

Table 4-6 LABEL

Function	Header	Query	Contents
LABEL	LAB#string#	LAB?	Up to 48 characters Example:LAB#ABC-890#

Table 4-7 MEASURE

Function	Header	Query	Contents
MEASURE	MEA *	MEA?	0: STOP, 1: SINGLE, 2: REPEAT

4.10 GPIB Command Codes

Table 4-8 DISPLAY (1 of 5)

Function	Header	Query	Contents	
CONTROL	DUAL	DUA *	DUA?	0: OFF, 1: ON(Dual-screen)
	SUPER IMPOSE	SIM *	SIM?	0: OFF, 1: ON(Super-impose)
	GRID	GRI *	GRI?	0: OFF, 1: ON
	act.U&L	AUL *	AUL?	0: Upper screen active, 1: Both upper and lower screens active
	xcng U/L	XUL *	-	Switches between the upper and lower screens
	Sampling Point	SPT *	SPT?	0: 101, 1: 201, 2: 501, 3: 1001, 4: 2001, 5: 5001, 6:10001
	AUTO SAMPLE	ASP *	ASP?	0: OFF, 1: ON
CONTROL (MULTI TRACE)	MULTI TRACE ON/OFF	MTE *	MTE?	0: OFF, 1: ON
	TRACE MAX	MMX *	MMX?	Setting the maximum number of traces, Range: 1 to 32
	NEXT TRACE	MNT	-	Selecting the nest trace number.
	PREVIOUS TRACE	MPT	-	Selecting the previous trace number.
	CURRENT TRACE SET	MCU *	MCU	Selecting a trace number, Range: 1 to MMX
	AUTO TRACE INCREMENT	MAT *	MAT	0: OFF, 1: ON
	DELETE CURRENT TRACE	MDC	-	Clearing the waveform data of the current trace number.
	DELETE ALL TRACE	MDA	-	Clearing all waveform data.
SAVE	SAVE MEAS DATA	SAV#file name#	-	#REF#: Saves into memory as reference data. #MEAS1#: Saves into memory MEAS1. #MEAS2#: Saves into memory MEAS2. #MEAS3#: Saves into memory MEAS3. #file name#: Saves into memory or FD. Example:SAV#LD123#
	DELETE MEAS	DMD#file name#	-	#file name#: Deletes data into memory or FD. Example:DMD#1550LD#

Table 4-8 DISPLAY (2 of 5)

Function		Header	Query	Contents
RECALL	RECALL MEAS	RCL#file name#	-	#REF#: Recalls data from the reference data memory. #MEAS1#: Recalls data from MEAS1. #MEAS2#: Recalls data from MEAS2. #MEAS3#: Recalls data from MEAS3. #file name#: Recalls data from memory or FD. Example:RCL#MEAS1#
PEAK NORMALIZE		PNR *	PNR?	0: OFF, 1: ON(Peak normalize)
LOSS		LOS *	LOS?	0: OFF, 1: ON
TRANS		TRA *	TRA?	0: OFF, 1: ON
ADVANCE (PEAK POWER MONITOR)	PEAK POWER MONITOR ON/OFF	PMO *	PMO?	0: OFF(Spectrum), 1: ON(Power Monitor)
	PEAK POWER MONITOR N-MAX	PNX *	PNX?	Integer(11 to 1001) Point of trend-chart
	PEAK POWER MONITOR INTERVAL	PIN *	PIN?	Numeric(0.5 to 3600) Measurement interval of power monitor [sec]
ADVANCE (LIMIT LINE)	PATTERN SELECT	LPT *	LPT?	Selecting LIMIT LINE ON/OFF and the pattern file. 0: LIMIT LINE OFF 1: Selecting a pattern file 1 to 5.
	LOAD PATTERN FILES	LPR	-	Loading a pattern file from a floppy disk.
APPLICATION (SPEC.WIDTH)	SPEC.WIDTH	SPW *	SPW?	0:OFF, 1:ON
	WIDTH TYPE	WTY *	WTY?	0:Pk-XdB, 1:Envelope, 2:RMS, 3:Peak RMS, 4:Xnm Level
	THRESHOLD LVL1	WPX *	WPX?	Setting range: -59.9 to 59.9
	THRESHOLD LVL2	WPY *	WPY?	Setting range: 0.1 to 99.9
	K parameter	WPK *	WPK?	K parameter setting (used for WTY2 and 3) Setting range: 0.1 to 100
	Kr(RMS) param	WPR *	WPR?	Setting range: 1 to 10
	Xnm Level	WPW *	WPW?	Unit UM; $\mu$ m, NM:nm(default setting)
(NOTCH WIDTH)	Notch Width	NWD *	NWD?	0:OFF, 1:XdB Width, 2:Xnm Level
	XdB Width(Notch)	NLV *	NLV?	Setting range: -59.9 to 59.9
	Xnm Level(Notch)	NWI *	NWI?	Unit UM; $\mu$ m, NM:nm(default setting)

4.10 GPIB Command Codes

Table 4-8 DISPLAY (3 of 5)

Function	Header	Query	Contents	
(OPT AMP)	Optical Amp ON/OFF	OAM *	OAM?	0:OFF, 1:ON
	Optical AMP Mode	OMD *	OMD?	0:Single, 1:WDM
	NF(s-sp) or NF(total)	NFT *	NFT?	0:NF(s-sp), 1:NF(total)
	Spectrum Division	SDV *	SDV?	0:OFF, 1:ON
	K parameter (OPT AMP)	NFK *	NFK?	K parameter setting Setting range: 0.1 to 100
	Filter $\Delta\lambda$	FDL *	FDL?	Unit UM: $\mu\text{m}$ , NM:nm(default setting)
	Pin LOSS	LPI *	LPI?	Measuring system input loss setting (-10 to +10)
	Pout LOSS	LPO *	LPO?	Measuring system output loss setting (-10 to +10)
	Select Pin	NPK *	NPK?	0: OFF (displayed data or REF data) 1: ON (set using PLV)
	Select Level	PLV *	PLV?	Setting the input level used for NPK1, Unit DBM:dBm (as the initial value), MW:mW, UW: $\mu\text{W}$ , NW: nW
	Set Pin Wavelength	PLW *	PLW?	Setting the center wavelength used for NPK1, Unit UM: $\mu\text{m}$ , NM: nm (as the initial value)
(WDM LIST)	WDM LIST ON/OFF	WDM *	WDM?	0:OFF, 1:ON
	WDM Mode	WMD *	WMD?	0:Multi Peak, 1:SNR, 2:Relative, 3:ITU GRID
	WDM Ref. GH Select	WRF *	WRF?	Setting the reference channel number in the WDM list function.
	GRID ref. Frequency	GRF *	GRF?	WMD3 reference frequency setting Unit THZ:THz(default setting), GHZ:GHz
	GRID CH Spacing	GSP *	GSP?	WMD3 CH spacing frequency setting Unit THZ:THz, GHZ:GHz(default setting)
	ASE NBW Select	SRS *	SRS?	Sets whether the current or calculated value is used for the WMD1 ASE level. 0:Current, 1:Conversion
	ASE Conversion NBW	SCR *	SCR?	SRS1 wavelength resolution setting using the calculated value Unit UM: $\mu\text{m}$ , NM:nm(default setting)
	LIST ALL	WAL *	WAL?	0: OFF, 1: ON

Table 4-8 DISPLAY (4 of 5)

	Function	Header	Query	Contents
(WDM MONI-TOR)	WDM MONIT ON/OFF	LTM *	LTM?	0: OFF, 1: ON
	SPECTRUM display	LSD *	LSD?	0: OFF, 1: ON
	GRAPH X	LHA *	LHA?	0: Time, 1: CH No.
	DATA MODE	LVA *	LVA?	0: Wavelength/Frequency, 1: Level, 2: SNR
	ABSOLUTE/RELATIVE	LAR *	LAR?	0: Absolute value, 1: Relative value to the initial value, 2: Relative value to the nominal value
	Graph All Data	LDA *	LDA?	0: OFF, 1: ON
	Current Time No.	LCT *	LCT?	Setting the reference time number. Example: LCT101
	Current Channel No.	LCC *	LCC?	Setting the reference channel number, Example: LCC256
	Measurement Times	LMT *	LMT?	Number of measurements (1 to 501)
	Time Interval	LTl *	LTl?	Measurement interval [Min] (0.1 to 1440), Example: LT160
	Limit Judge Enable	LTF *	LTF?	0: OFF, 1: ON
	$\lambda$ drift Lmt.	LFD *	LFD?	Drift limit wavelength from ITU GRID when LTF1 is set to 1, Unit UM: $\mu$ m, NM: nm (as the initial value)
	Nominal Level	LNL *	LNL?	Reference power level when LAR2, Unit DBM: dBm (as the initial value), MW:mW, UW: $\mu$ W, NW: nW
	Level Upper Lmt.	LUL *	LUL?	Maximum power limit when LTF1, Unit DBM: dBm (as the initial value), MW:mW, UW: $\mu$ W, NW: nW
	Level Lower Lmt.	LLL *	LLL?	Minimum power limit when LTF1, Unit DBM: dBm (as the initial value), MW:mW, UW: $\mu$ W, NW: nW
	Nominal SNR	LNS *	LNS?	Reference SNR value [dB] when LAR2, Range: 0 to 60
SNR Lower Lmt.	LSL *	LSL?	Minimum SNR limit value [dB] when LTF1 is set to 1, Range: 0 to 60	

4.10 GPIB Command Codes

Table 4-8 DISPLAY (5 of 5)

Function	Header	Query	Contents	
(OPT AMP, WDM LIST, WDM MONI- TOR)	WDM THRESHOLD LEVEL	WYD *	WYD?	Threshold level (from the peak) setting used to detect the WDM signal Setting range: 0.1 to 99.9
	WDM ASE Method	WAU *	WAU?	ASE automatic detection function when set to OMD1 or WDM1. 0:AUTO OFF, 1:AUTO ON
	ASE Fitting	FTM *	FTM?	Selecting an interpolation curve when not set to ASE AUTO. 0:GAUSS,1:FIT MEM3, 2:Manual ASE
	Manual ASE Level	MAL *	MAL?	ASE level setting for FTM2 Unit DBM:dBm(default setting), MW:mW, UW:μW, NW:nW
	Masked SPAN	SNA *	SNA?	Setting ASE interpolation range "A" for FTM 0 and FTM 1 Unit UM:μm, NM:nm(default setting)
	Fitting SPAN	SNB *	SNB?	Setting ASE interpolation range "B" for FTM 0 and FTM 1 Unit UM:μm, NM:nm(default setting)



Table 4-9 DATA OUT

Function		Header	Query	Contents
DEVICE	DEVICE TYPE	DEV *	DEV?	0: Internal printer, 1: External printer, 2: Floppy disk
	FLOPPY ON/OFF	FON *	FON?	0: FLOPPY-OFF(MEMORY), 1: FLOPPY-ON
	FLOPPY FORMATTING	FFO *	-	1: 2DD(720K), 2: 2HD(1.44M)
	Bitmap Compless	BCP *	BCP?	0: Compress OFF, 1: Compress ON
	Bitmap Save	BSV *	BSV?	0: B&W, 1: Gray, 2: Color Bitmap
	EXT KEY	EKB *	EKB?	External keyboard settings 0: US, 1: JP
	Color Pattern	CPT *	CPT?	0 to 4 Selecting color patterns
	Ext. PRT MODE	EPM *	EPM?	0: GRAY, 1:B&W-S, 2: B&W-L
	Ext. PRT COMMAND	PRT *	PRT?	0: ESC/P, 1: ESC/P RAS, 2: HP PCL
	BUZZER(BEEP)	BUZ *	BUZ?	0: OFF, 1: ON
	WARNING	WAR *	WAR?	0: OFF, 1: ON
	QUIET BEEP	QUI *	QUI?	0: NORMAL, 1: QUIET
	CLOCK	CLO #YY-MM- DD,hh:mm:ss#	CLO?	-
	CLOCK ON/OFF	CKD *	CKD?	0: OFF, 1: ON
MENU OUT(printer)	MEN *	MEN?	0: OFF, 1: ON	
COPY		COP	-	Start outputting to selecting device by DEVICE TYPE
FEED		FEE	-	Paper fed about 5 mm to printer. (Internal printer)

## 4.10 GPIB Command Codes

Table 4-10 Codes Corresponding to Other Keys

Function		Header	Query	Contents
INSTR PRESET		IPR	-	Measurement conditions initialized.
CAL	CAL $\lambda$ (Int.)	CLM	-	
	CAL $\lambda$ (Ext.)	CLE *	CLE?	Unit UM: $\mu$ m, NM:nm(default setting)
	$\lambda$ OFFSET	CLF *	CLF?	Unit UM: $\mu$ m, NM:nm(default setting)
	LEVEL OFFSET	CLS *	CLS?	Unit DB:dB(default setting)
	AUTO ALIGNMENT	ALM	-	-

Table 4-11 Controlling Data Output and Others (1 of 3)

Function	Header	Query	Contents
SRQ signal control-1	SRQ *	SRQ?	0: Mode not transmitting SRQ, 1: Mode transmitting SRQ
SRQ signal control-2	S *	S?	0: Mode transmitting SRQ, 1: Mode not transmitting SRQ
Status byte mask	MSK *	MSK?	0 to 255 (Bit 6 can not be masked.) Status byte bit "1" to be masked switched on. (Initial value: 0)
Status byte clear	CSB	-	
Header data output control	HED(HD) *	HED?	0: HEADER OFF, 1: HEADER ON
Terminator	DEL(DL) *	DEL?	0: NL<EOI>, 1: NL, 2: <EOI>, 3: CR NL<EOI>
Data separator	SDL(DS) *	SDL?	0: ,(comma), 1: SP(space), 2: CR NL
Message separator	MSP(MS) *	MSP?	0: ,(semicolon), 1: CR NL
Data output format (valid for waveform data)	FMT *	FMT?	0: ASCII, 1: BINARY(16bit), 2: BINARY(64bit float), 3: BINARY(32bit float), 4: BINARY(32bit float NEC)
Data output screen	OVS *	OVS?	0: upper(upper screen), 1: lower(lower screen)
Request for waveform data output	OSD *	-	0: Y-axis data output, 1: X-axis data output, 2: Outputs Y-axis data for MIN HOLD, 3: Outputs Y-axis data for MAX HOLD
Request for output of the number of waveform data	ODN	ODN?	Output of the number of data contained on the screen specified by OVS <sub>n</sub> or trend-chart
Request for peak search data output	OPK	OPK?	-

Table 4-11 Controlling Data Output and Others (2 of 3)

Function	Header	Query	Contents
Request for cursor data output	OCD	OCD?	Output data differs depending on cursor display mode.
Request for spectral width data output	OSW	OSW?	Output of the spectral width calculated
Output of notch width data	ONW	ONW?	Output of the notch width calculated
Request for operation result of gain and noise figure	OGN	OGN?	Output of gain and noise figure calculated.
Request for power monitor data output	OPM	OPM?	Output of point data measured by power monitor
Request for outputting operation results of gain, noise figure and total ASE power	OPN	OPN?	Output of gain, noise figure and total ASE power calculated.
WDM PEAK NO	OWP	OWP?	Number of WDM signal lights that have been measured using the NF command.
Request for outputting number of list data	OLN	OLN?	Number of optical signals in the WDM list
Request for outputting operation results of WDM	OLS	OLS?	Request to output data consisting of Multi Peak, SNR and Relative ITV GRID that have been selected using NF data (obtained from WDM operation) or WDM LIST operation.
Request for WDM gain noise in real type	OWN	OWN?	Adding Pout output to OLS.
Request for outputting start point at the X axis of the ASE fitted data	PAS	PAS?	Output of start point at the X axis of the ASE fitted data in gain or WDM operation.
Request for outputting the number of ASE fitted data	PAN	PAN?	Output of the number of ASE fitted data in gain or WDM operation.
Request for outputting ASE fitted data	OPA	OPA?	Output of ASE fitted data in gain or WDM operation
Request for data from the WDM monitor	OLT*	-	Outputs the nth time data for each channel using OLTn.
Outputs the number of WDM MONITOR time data sets	ONT	ONT?	
Request for LIMIT judgment results of the WDM monitor function	LRS	LRS?	0: FAIL 1: PASS
Request for LIMIT judgment results of the LIMIT LINE function	LPF	LPF?	0: FAIL 1: PASS
Single measurement	E(*TRG)	-	Code identical to "MEA1" Single measurement executed

4.10 GPIB Command Codes

**Table 4-11 Controlling Data Output and Others (3 of 3)**

Function	Header	Query	Contents
Initialization	C(*RST)	-	Resets the parameter values to the factory defaults.
Device identification	-	*IDN?	Request to output company name, device name, serial number and software revision.
Execution of self-diagnosis and output of results.	*TST	*TST?	Request to execute the self-diagnosis and output the results.

**Table 4-12 Error Codes Associated with the Self-diagnosis Function**

Code	Description
0000	Normal
XXX1	Decimal place: Analysis board error
XX1X	Tens place: Backup RAM error
X1XX	Hundreds place: Measurement error
1XXX	Thousands place: Error in the optional light source for calibration

## 4.11 Example Programs

This section describes remote control examples used with GPIB port.

### 4.11.1 Sample Programs for Setting or Reading Measurement Conditions

---

**CAUTION:** *Visual Basic 4.0 (referred to as VB henceforth) is used in the sample programs shown here. Also, National Instruments-made GPIB board (referred to as NI-made for brevity henceforth) is used for the GPIB control board; NI-made driver is used for the control driver.*

---

- Program examples using VB

Example VB-1: Setting the center wavelength after performing an analyzer master reset

```
Call ibclr(spa)                'Performs a Device Clear.
Call ibwrt(spa,"C")           'Preset
Call ibwrt(spa,"CEN1550nm")   'Set the center wavelength to 1550 nm.
Call ibwrt(spa,"SPA20nm")     'Set the span to 20 nm.
```

Example VB-2: After the center wavelength, span and so on have been set, the peak wavelength and level are read. (SRQ is used.)

```
Dim boardID As Integer
Dim res As Integer
Dim Peak_lambda#, Peak_Level#

boardID = 0

Call ibclr(spa)                'Performs a Device Clear.

Call ibwrt(spa,"C")           'Preset
Call ibwrt(spa,"CEN1550nm,SPA20nm") 'Set the center wavelength to 1550 nm and the span to 20 nm.
Call ibwrt(spa,"REF0dBm")     'Set the reference level to 0 dBm.
Call ibwrt(spa,"LIN0,LEV0")   'Set the LOG display to 10 dB/DIV.
Call ibwrt(spa,"SWE1,RES0.1nm") 'Set the sweep mode to ADAPTIVE and the resolution to 0.1 nm.
Call ibwrt(spa,"MSK254")     'Enable measurement-end of status byte (b0)
Call ibwrt(spa,"SRQ1")       'Enable SRQ interrupt
Call ibwrt(spa,"MEAL")       'Start single measurement

Call ibwait(spa,RQS Or TIMO)  'Waiting for SRQ interrupt
Call ibrsp(spa,res)          'Read the status byte

Call ibwrt(spa,"DEL0,SDL2,HED0") 'Set the delimiter and the output header to OFF
Call ibwrt(spa,"OPK")        'Output of peak search data is requested.

Rdbuf = Space(15)            'Allocate a maximum of 15 bytes, including delimiters.
Call ibrd(spa,Rdbuf)         'Read the peak search data (wavelength).
Peak_lambda = Val(Rdbuf)     'Convert ASCII format into numeric values.
Rdbuf = Space(12)            'Allocate a maximum of 12 bytes, including delimiters.
Call ibrd(spa,Rdbuf)         'Read the peak search data (level).
Peak_Level = Val(Rdbuf)     'Convert ASCII format into numeric values.
```

4.11 Example Programs

Example VB-3: Center wavelength and span are set for spectrum analysis and peak wavelength and level are read. (SRQ is not used.)

```

Dim res As Integer

Call ibclr(spa) 'Performs a Device Clear.

Call ibwrt(spa,"C") 'Preset
Call ibwrt(spa,"STA1220nm,SOP1400nm") 'Set the center wavelength to 1220 nm and the stop wavelength to 1400 nm.

Call ibwrt(spa,"REF0.1mW") 'Set the reference level to 0.1 mW.
Call ibwrt(spa,"SWE2,RES0.5nm") 'Set the sweep mode to HI-SENS1 and the resolution to 0.5 nm.
Call ibwrt(spa,"AVG2") 'Averaging is set to 2.
Call ibwrt(spa,"MSK254") 'Enable measurement-end of status byte (b0)
Call ibwrt(spa,"CSB") 'Clear the status byte.
Call ibwrt(spa,"MEA1") 'Start single measurement.
Do
    Call ibrsp(spa,res) 'Read the status byte.
    DoEvent 'Check for other events occurring in the loop.
Loop Until(res AND 1) 'Exit from the loop if the measurement end bit is set.

Call ibwrt(spa,"DEL0,SDL2,HED0") 'Set the delimiter and the output header to OFF
Call ibwrt(spa,"OPK") 'Output of peak search data is requested.

Rdbuff = Space(15) 'Allocate a maximum of 15 bytes, including delimiters.
Call ibrd(spa,Rdbuff) 'Read the peak search data (wavelength).
Peak_lambda = Val(Rdbuff) 'Convert ASCII format into numeric values.
Rdbuff = Space(12) 'Allocate a maximum of 12 bytes, including delimiters.
Call ibrd(spa,Rdbuff) 'Read the peak search data (level).
Peak_Level = Val(Rdbuff) 'Convert ASCII format into numeric values.
    
```

Example VB-4: After setting measurement conditions for spectrum analysis, the spectrum data obtained is read in the ASCII format.

```

Dim i%, n%, res%
Dim Rdbuff As String
Dim spLev() As String, spLen() As String
Dim spLevel() As Double, spLength() As Double

Call ibclr(spa) 'Performs a Device Clear.

Call ibwrt(spa,"C") 'Preset
Call ibwrt(spa,"CEN1550nm,SPA20nm") 'Set the center wavelength to 1550 nm and the span to 20 nm.
Call ibwrt(spa,"REF0dBm") 'Set the reference level to 0 dBm.
Call ibwrt(spa,"SWE1,RES0.1nm") 'Set the sweep mode to ADAPTIVE and the resolution to 0.1 nm.
Call ibwrt(spa,"MSK254") 'Enable measurement-end of status byte (b0).
Call ibwrt(spa,"SRQ1") 'Enable SRQ interrupt

Call ibwrt(spa,"MEA1") 'Start single measurement.
Call ibwait(spa,RQS Or TIMO) 'Waiting for SRQ interrupt.
Call ibrsp(spa,res) 'Read the status byte.

Call ibwrt(spa,"FMT0,HED0,SDL2") 'Set the ASCII format and the delimiter. Data output of header is set to OFF.
Call ibwrt(spa,"ODN") 'Output of data number is requested.

Rdbuff = Space(8) 'Allocate a maximum of 8 bytes, including delimiters.
Call ibrd(spa,Rdbuff) 'Read the number of data.
n = Val(Rdbuff) 'Convert ASCII format into numeric values.
    
```

```

ReDim spLev(n), spLen(n)
ReDim spLevel(n), spLength(n)

Call ibwrt(spa, "OSD0")
For i = 1 To n
    spLev(i) = Space(13)
    Call ibrd(spa, spLev(i))
    DoEvents
Next i
Call ibwrt(spa, "OSD1")
For i = 1 To n
    spLen(i) = Space(15)
    Call ibrd(spa, spLen(i))
    DoEvents
Next i
For i = 1 To 10
    spLevel(i) = Val(spLev(i))
    spLength(i) = Val(spLen(i))
Next i

```

'Request the wavelength data (vertical axis)  
'Allocate a maximum of 13 bytes, including delimiters.  
'Read the level data.  
'Check for other events occurring in the loop.  
'Request the wavelength data (horizontal axis)  
'Allocate a maximum of 15 bytes, including delimiters.  
'Read the wavelength data.  
'Check for other events occurring in the loop.  
'Convert ASCII format into numeric values.  
'Convert ASCII format into numeric values.

**Example VB-5:** After setting measurement conditions for spectrum analysis, the spectrum data obtained is read in the binary format.

```

Dim i%, n%, res%
Dim Rdbuff As String
Dim d1%, d2%, d3%, d4%
Dim si#, de#, dk#
Dim spLev() As Integer, spLen() As Integer
Dim spLevel() As Double, spLength() As Double

Call ibclr(spa)
Call ibwrt(spa, "C")
Call ibwrt(spa, "CEN1550nm, SPA20nm")
Call ibwrt(spa, "REF0dBm")
Call ibwrt(spa, "SWE1, RES0.1nm")
Call ibwrt(spa, "MSK254")
Call ibwrt(spa, "SRQ1")
Call ibwrt(spa, "MEA1")

Call ibwait(spa, RQS Or TIMO)
Call ibrsp(spa, res)

Call ibwrt(spa, "FMT3, HED0, SDL2")

Call ibwrt(spa, "ODN")

Rdbuff = Space(8)
Call ibrd(spa, Rdbuff)
n = Val(Rdbuff)

ReDim spLev(n * 4 / 2 - 1), spLen(n * 4 / 2 - 1)
ReDim spLevel(n), spLength(n)

Call ibconfig(spa, IbcReadAdjst, 1)
Call ibwrt(spa, "OSD0, DEL2")

Call ibrdi(spa, spLev(), n * 4)

```

'Performs a Device Clear.  
'Preset  
'Set the center wavelength to 1550 nm and the span to 20 nm.  
'Set the reference level to 0 dBm.  
'Set the sweep mode to ADAPTIVE and the resolution to 0.1 nm.  
'Enable measurement-end of status byte (b0).  
'Enable SRQ interrupt  
'Start single measurement.  
'Waiting for SRQ interrupt.  
'Read the status byte.  
'Set the binary format and the delimiter. Data output of header is set to OFF.  
'Output of data number is requested.  
'Allocate a maximum of 8 bytes, including delimiters.  
'Read the number of data.  
'Convert ASCII format into numeric values.  
'Perform the byte swapping when reading it.  
'Request the wavelength data (horizontal axis) as output data, and specify EOI for the delimiter.  
'Read the wavelength data.

## 4.11 Example Programs

```

*****
'Convert the binary data into the numeric data (wavelength data).
*****
For i = 1 To n
  If spLev((i - 1) * 2 + 0) > 0 Then
    d1 = spLev((i - 1) * 2 + 0) \ 256
    d2 = spLev((i - 1) * 2 + 0) Mod 256
  Else
    d1 = (65536 + spLev((i - 1) * 2 + 0)) \ 256
    d2 = (65536 + spLev((i - 1) * 2 + 0)) Mod 256
  End If
  If spLev((i - 1) * 2 + 1) > 0 Then
    d3 = spLev((i - 1) * 2 + 1) \ 256
    d4 = spLev((i - 1) * 2 + 1) Mod 256
  Else
    d3 = (65536 + spLev((i - 1) * 2 + 1)) \ 256
    d4 = (65536 + spLev((i - 1) * 2 + 1)) Mod 256
  End If
  If d1 > 127 Then
    si = -1
    de = (d1 - 128#) * 2# + (d2 \ 128)
  Else
    si = 1
    de = d1 * 2# + (d2 \ 128)
  End If
  If d2 > 127 Then
    dk = (d4 + d3 * 256# + d2 * 65536#) / 8388608#
  Else
    dk = (d4 + d3 * 256# + (d2 + 128#) * 65536#) / 8388608#
  End If
  spLevel(i) = si * (2 ^ (de - 127)) * dk
Next i

Call ibwrt(spa, "OSD1,DEL2")           'Request the level data (vertical axis)
Call ibrdi(spa, spLen(), n * 4)       'Read the level data.

*****
'Convert the binary data into the numeric data (level data).
*****
For i = 1 To n
  If spLen((i - 1) * 2 + 0) > 0 Then
    d1 = spLen((i - 1) * 2 + 0) \ 256
    d2 = spLen((i - 1) * 2 + 0) Mod 256
  Else
    d1 = (65536 + spLen((i - 1) * 2 + 0)) \ 256
    d2 = (65536 + spLen((i - 1) * 2 + 0)) Mod 256
  End If
  If spLen((i - 1) * 2 + 1) > 0 Then
    d3 = spLen((i - 1) * 2 + 1) \ 256
    d4 = spLen((i - 1) * 2 + 1) Mod 256
  Else
    d3 = (65536 + spLen((i - 1) * 2 + 1)) \ 256
    d4 = (65536 + spLen((i - 1) * 2 + 1)) Mod 256
  End If
  If d1 > 127 Then
    si = -1
    de = (d1 - 128#) * 2# + (d2 \ 128)
  Else
    si = 1
    de = d1 * 2# + (d2 \ 128)
  End If

```



```
If d2 > 127 Then
    dk = (d4 + d3 * 256# + d2 * 65536#) / 8388608#
Else
    dk = (d4 + d3 * 256# + (d2 + 128#) * 65536#) / 8388608#
End If
spLength(i) = si * (2 ^ (de - 127)) * dk
Next i
Call ibconfig(spa, IbcReadAdjust, 0)      'Cancel the byte swapping when reading it.
```

## 5 TECHNICAL NOTES

### 5.1 Measurement Modes

There are six measurement modes (sweep modes) available which can be used to measure a variety of optical signals in this optical spectrum analyzer. Measuring time or the minimum measurable level (or sensitivity) varies depending on the measurement mode used. As a result, choose the appropriate mode for the optical signal used.

- **NORMAL**  
Measures relatively high-level optical signals at high speeds.
- **ADAPTIVE**  
Measures signals which require relatively high sensitivity at relatively high speeds. This mode is also used to measure optical signals from pulsing emission in sync with an external signal.
- **ADAPTIVE (Pulsing optical signals: External sync mode)**  
Measures pulsed optical signals which are input to the GATE MEAS INPUT connector in sync with an external signal.

This input level has a logic level of TTL.

The externally synchronized measurement function automatically starts when a pulse signal is detected at the GATED MEAS INPUT terminal when the measurement is set to ADAPTIVE. When this input is not used, its level is considered HIGH because it is internally pulled up. Use a synchronization signal with a constant period.

There are two modes for the externally synchronized measurement function: SYNC LOW and SYNC HI.

- **SYNC LOW Mode**  
An AD sampling is performed with the high level of a synchronization signal.  
Minimum optical pulse width: 10 nsec (30  $\mu$ sec or more is recommended).  
A pulse width of 30  $\mu$ sec or less is displayed a little lower than the actual level.  
The internal optical detector has a bandwidth of approximately 10 kHz and the sensitivity is approximately 10 dB lower than the normal sensitivity in ADAPTIVE Mode.
- **SYNC HI Mode**  
An AD sampling is performed at less than 1000  $\mu$ sec (specified by "Delay Time") after the specified rising or falling edge parameter of the synchronization signal is detected.  
The internal optical detector has a bandwidth of approximately 1 MHz and the sensitivity is approximately 40 dB lower than the normal sensitivity in ADAPTIVE Mode.
- **HI DYNAMIC1/2**  
Used to measure optical signals so that the dynamic range is larger than the range used in ADAPTIVE mode by intercepting the stray light caused by the monochromator.  
The HI DYNAMIC2 has a larger dynamic range than HI DYNAMIC1.
- **HI-SENSE1/2**  
A higher priority is given to the sensitivity.  
HI-SENSE2 has a higher sensitivity than HISENSE1.

5.2 Averaging Functions

- PULSE (Peak Hold Mode)

A pulse optical measurement is made using the internal peak hold circuitry without using an external synchronization signal. The peak hold circuitry performs an AD sampling for the peak level of a pulse signal that is held during GATE TIME. As a result, "GATE TIME" must be longer than the input optical pulse period.

The internal optical detector has a bandwidth of approximately 10 kHz so that the measurement level is lower than actual level when an optical signal whose pulse width is 30 μsec or less.

The sensitivity is approximately 20 dB lower than the normal sensitivity in ADAPTIVE Mode.

When GATE TIME is set to 0, the built-in low-pass filter is connected instead of the peak hold circuitry, and the average power level of the optical signal is measured.

**Table 5-1 Throughput, Sensitivity and Dynamic Range for Each Measurement Mode at a Wavelength of 1.55 μm (typical value)**

	NORMAL	ADAPTIVE	Hi Sens 1	Hi Sens 2	Hi Dyna 1	Hi Dyna 2
Span 50 nm, 501 point	0.5 sec	3.5 sec	28 sec	55 sec	9.0 sec	50 sec
Span 50 nm, 1001 point	0.9 sec	4.5 sec	60 sec	110 sec	17 sec	100 sec
Sensitivity (1.5 μm typical value)	-65 dBm	-73 dBm	-88 dBm	-90 dBm	-74 dBm	-87 dBm
Dynamic range		+	+	+	++	++

**5.2 Averaging Functions**

The optical spectrum analyzer is equipped with the mode of noise reduction which can measure low-level optical signals.

- Point Average

Displays a spectrum with reduced noise after one sweep: takes data at each measurement point the specified number of times, and then performs averaging for each point.

- Sweep average

Performs sweeps repetitively, and performs averaging for each point. Noise is reduced as the number of sweeps increases.

- Smoothing

Performs averaging by assigning weights to the adjacent points to smooth the measurement waveform.

### 5.3 Calculating the Spectral Width and the Notch Width

There are five modes available for calculating spectral width using this optical spectrum analyzer. Notch widths can also be calculated. The center wavelength, spectral width and the number of peaks are displayed after each calculation. The description for each method is shown below.

If two X cursors are displayed, the section between the two cursors is calculated.


#### 5.3.1 Calculating the Spectral Width

##### 5.3.1.1 PEAK THRESHOLD

The spectral width and center wavelength can be calculated from two intersections of the level line *THRESHOLD LVL1* below the maximum peak and two lines obtained using the linear interpolation.


The linear interpolation is performed using the LOG or LIN scale coordinates.

If a negative value is assigned to *THRESHOLD LVL1*, the level is increased by the value above the minimum level.

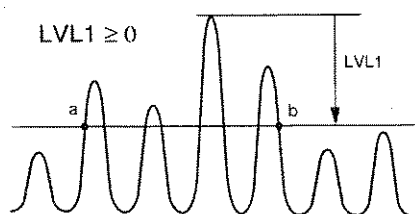

$$\lambda_0 = \frac{\lambda_a + \lambda_b}{2}$$

$$\Delta\lambda = \lambda_b - \lambda_a$$

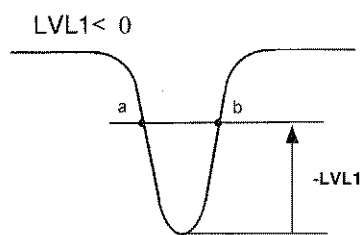

$$\lambda_0 = \frac{\lambda_a + \lambda_b}{2}$$

$$\Delta\lambda = \lambda_b - \lambda_a$$


5.3 Calculating the Spectral Width and the Notch Width

5.3.1.2 ENVELOPE

Creates an envelope of monotonous peak from the peaks whose levels are above the line a level specified by **THRESHOLD LVL 2** below the maximum peak. The spectral width and center wavelength are calculated from the points where the line a level specified by **THRESHOLD LVL1** below the maximum peak (for LVL 1 ≥ 0).

The linear interpolation is performed using the LOG or LIN scale coordinates.


If there are no peaks whose values are above the level THRESHOLD LVL2 below the maximum peak, the result is 0 because no envelope has been obtained.

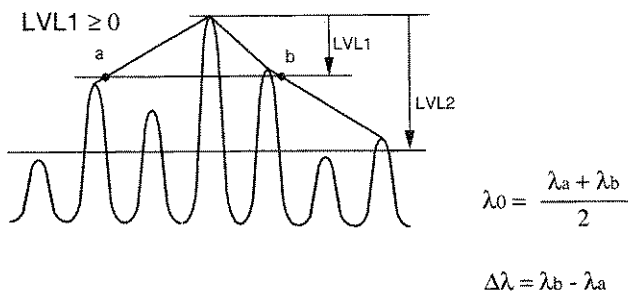

5.3.1.3 RMS

The center wavelength is calculated from the weighted average of all spectrums displayed. The spectral width is the product of the standard deviation for the wavelength and  $K_r(\text{RMS})$  that has previously been set.


The initial value of K is 1, and the initial value of  $K_{\text{RMS}}$  is 2.3548.

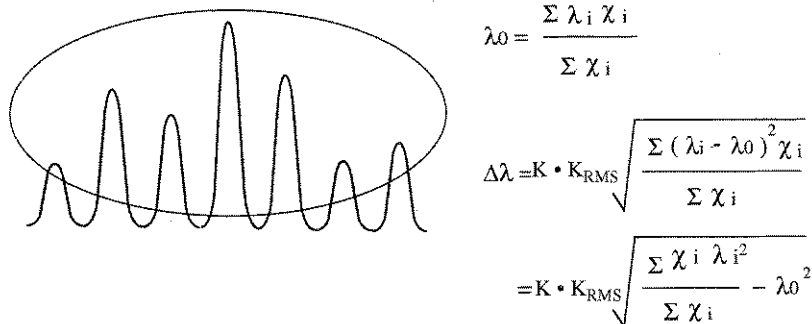

### 5.3.1.4 Peak RMS


The center wavelength is calculated using the weighted average method for the wavelength of each peak whose level is above the line a level specified by **THRESHOLD LVL 2** below the maximum peak. The spectral width for each peak is the product of the standard deviation for the wavelength and constant  $K_r(\text{RMS})$ .

The initial value of  $K$  is 1, and the initial value of  $K_{\text{RMS}}$  is 2.3548.

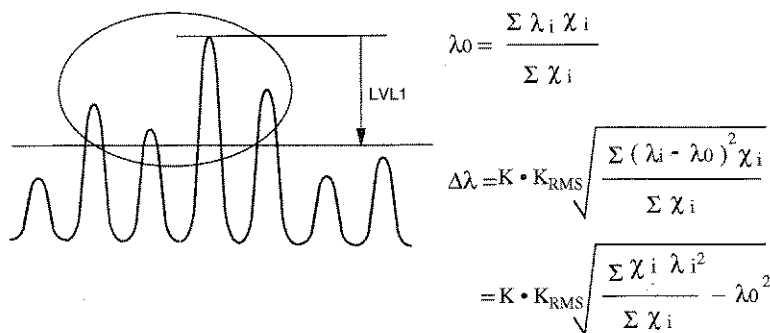

### 5.3.1.5 Xnm Level

Calculates the level difference between the maximum peak and the level whose spectrum width is Xnm.

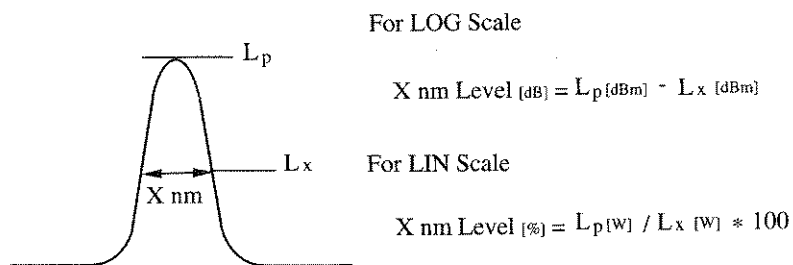


5.3 Calculating the Spectral Width and the Notch Width

5.3.2 Notch Width


5.3.2.1 XdB WIDTH

The notch width and center wavelength are calculated from the points where the line a level specified by **THRESHOLD LVL1** below the maximum peak (for LVL1 ≥ 0). The linear interpolation is performed using the LOG or LIN scale coordinates.

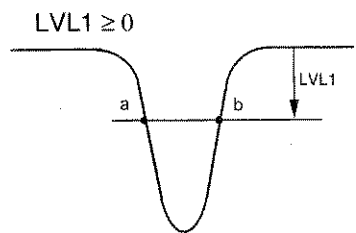

$$\lambda_0 = \frac{\lambda_a + \lambda_b}{2}$$

$$\Delta\lambda = \lambda_b - \lambda_a$$

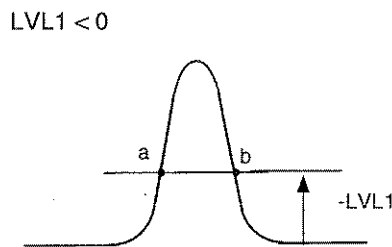

$$\lambda_0 = \frac{\lambda_a + \lambda_b}{2}$$

$$\Delta\lambda = \lambda_b - \lambda_a$$

LVL1 ≥ 0


The notch width is the difference between intersections a and b of the line XdB below the maximum level and the spectrum (the left and right intersections are referred to as a and b, respectively). The center wavelength is the midpoint between a and b.

LVL1 < 0

The notch width is the difference between intersections a and b of the line XdB above the minimum level and the spectrum (the left and right intersections are referred to as a and b, respectively). The center wavelength is the midpoint between a and b.

### 5.3.2.2 Xnm Level

Calculates the difference between the minimum level and the level whose spectrum width is Xnm.

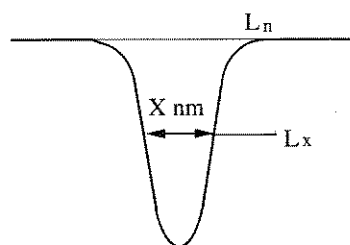

For LOG Scale

$$X \text{ nm Level (dB)} = L_n(\text{dBm}) - L_x(\text{dBm})$$

For LIN Scale

$$X \text{ nm Level (\%)} = L_n(\text{W}) / L_x(\text{W}) * 100$$



### 5.4 GAIN&NF and SNR

The optical spectrum analyzer calculates the noise figure characteristics and SNR of an optical amplifier after the amplified spontaneous emission (ASE) level has been calculated using the interpolation.

- The method of determining the ASE level using the ASE Fitting settings changes when WDM ASE Method is set to AUTO OFF, or when the Opt. AMP function is set to SNG mode.

(1) When ASE Fitting is set to Gauss mode


The level at the center wavelength for each signal is defined as the ASE level, and is calculated using a simulated Gaussian curve fitted to the two target sections (thick lines). These sections are calculated with Fitting SPAN and Masked SPAN.

(2) When ASE Fitting is set to MEM-3 mode

The level at the center wavelength for each signal is defined as the ASE level, and is calculated using the spectrum which was saved in MEAS 3 (memory 3) and then fitted to the two target sections (thick lines). These sections are calculated with Fitting SPAN and Masked SPAN.

(3) When ASE Fitting is set to Manual mode


Set Manual ASE LEVEL to the amplified spontaneous emission (ASE) level.

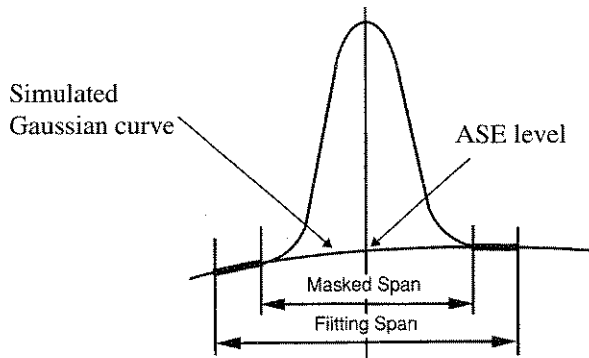

- When WDM ASE Method is set to AUTO ON, and the Opt. AMP function is not set to SNG Mode  
The lowest level between WDM signals is defined as the ASE level. The method of calculating the ASE level changes according to the number of WDM signals

**Table 5-2 Number of Signals and Interpolation Method.**

Number of signals	Processing
1 to 8	Calculates a simulated Gaussian curve based on the lowest level between adjacent valleys of a channel. The ASE level for each channel is defined as the level at the intersection point obtained as follows: a line that starts from the peak of the channel, descends perpendicular to the X-axis and intersects the simulated Gaussian curve.
9 or more	The line that connects adjacent lowest levels of a channel must first be determined. The ASE level for a channel is then defined as the level at the intersection point obtained as follows: a line which starts from the peak of the channel, descends perpendicular to the X-axis and intersects the lowest level line.

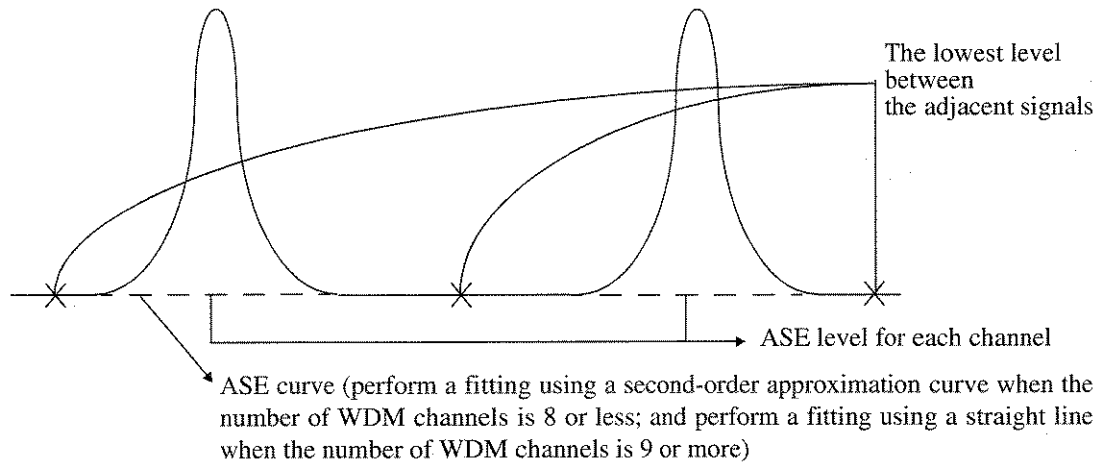

### 5.4.1 GAIN

The gain of the optical amplifier is calculated by using the formula shown below with the input and output optical levels and the ASE level that are previously calculated.

$$G = \frac{(P_{OUT} - P_{ASEM}) L_{OUT}}{P_{IN} L_{IN}}$$

## 5.4 GAIN&amp;NF and SNR

## 5.4.2 NF

The NF of the optical amplifier is calculated according to NF SELECT as shown below. Use the ASE and gain that have previously been obtained.

- When NF SELECT is set to total mode:

Terms 1 to 4 in the first formula are as follows:

Term1: Shot noise caused by an optical signal

Term2: Shot noise caused by an ASE

Term3: Beat noise between an optical signal and ASE

Term4: Beat noise between ASEs.

Set the parameter  $\Delta\lambda$  to the wavelength band of an optical receiver.

$$NF = K \left( \frac{1}{G} + \frac{2 \mu_x \Delta f}{G N} + 2 \mu_x + \frac{2 \mu_x^2 \Delta f}{N} \right)$$

$$N = \frac{P_{IN} L_{IN}}{h \nu}$$

$$\mu_x = \frac{P_{ASE}}{2 h \nu G \Delta \nu}$$

$$\Delta f = \frac{C}{\lambda_s - \Delta\lambda/2} - \frac{C}{\lambda_s + \Delta\lambda/2}$$

If  $\Delta\lambda$  is set to 0, NF is calculated using the formula below. This formula contains two terms related to the beat noise between the optical signal and spontaneous emission light, and the shot noise of the optical signal.

$$NF = K \left( \frac{P_{ASE}}{h \nu G \Delta \nu} + \frac{1}{G} \right)$$

- When NF SELECT is set to S-Sp mode

NF is calculated using the term related to the beat noise between the optical signal and spontaneous emission light only.

$$NF = K \frac{P_{ASE}}{h \nu G \Delta \nu}$$

G :	Gain
NF :	Noise Figure
P <sub>IN</sub> :	Input signal optical level (W)(measured value)
P <sub>OUT</sub> :	Output signal optical level (W)(measured value)
P <sub>ASEM</sub> :	ASE optical level before correction (W)
P <sub>ASE</sub> :	ASE optical level (W)
L <sub>IN</sub> :	"Pin Loss" value (setting value)
L <sub>OUT</sub> :	"Pout Loss" value (setting value)
K :	Coefficient for the calculation result (setting value)(initial value: 1.000)
C :	The velocity of signal light (2.9979*10 <sup>8</sup> [m/s])
N :	Photon number
h :	Plank's constant (6.63*10 <sup>-34</sup> [J s])
ν :	Signal light frequency (Hz)
Δν :	Frequency resolution during ASE measurement (Hz)
λ <sub>s</sub> :	Wavelength of signal light
Δλ :	Effective optical filtering width of optical amplifier output (setting value)

### 5.4.3 SPE DIV

To interpolate ASE level using the Opt.AMP function (which is used to calculate the noise factor of an optical amplifier), It is effective for high input levels of the optical amplifier (Saturation area).

When this mode is turned on, the correction spectrum (P<sub>CORR</sub>) is obtained from the output spectrum (P<sub>OUT</sub>) and input spectrum (P<sub>IN</sub>) using the following expression. The ASE level is calculated from the correction spectrum.

$$P_{CORR} = P_{OUT} - G \cdot P_{IN}$$

G: Gain at the signal light wavelength [G = (P<sub>OUT</sub> - P<sub>ASE</sub>)/P<sub>IN</sub>]

P<sub>ASE</sub>: Temporary ASE level obtained using fitting

When this mode is off, the ASE level can be obtained directly from the output spectrum.

## 5.5 Auto-Panning and Auto-Zooming Functions

### 5.5 Auto-Panning and Auto-Zooming Functions

The auto-panning and auto-zooming functions are used to interpolate or decimate measurement values automatically to match the number of sampling points when the number of sampling points or the conditions of the wavelength axis are changed.

These functions are performed under the following conditions:

- A change in the number of sampling points.
- A change in the center value or span of the wavelength axis.
- When the reference data and Loss/Trans data are measured under different conditions of the wavelength axis, the auto-panning or auto-zooming functions is performed for the reference data. (Refer to Section 2.2.6, "Measuring the Transmission-wavelength (or Loss-wavelength) Characteristics.")
- When the input and output signals of the amplifier are measured under different conditions of the wavelength axis to calculate the EDFA noise figure, the auto-panning and auto-zooming functions are performed for the input signal.

When the data is zoomed, data points are linearly interpolated.

When the data is panned, the excess data is unconditionally decimated.

## 5.6 Cursor Modes and Explanation for Displayed Data

The cursor modes and their display formats are as follows.

- NORMAL (when MAX HOLD and MIN HOLD are turned off)
  - $\lambda_1, I_1$ : Displays X cursor 1 wavelength, level
  - $\lambda_2, I_2$ : Displays X cursor 2 wavelength, level
  - L1, L2: Displays Y cursor 1, 2 level
- NORMAL (when MAX HOLD and MIN HOLD are turned on)
  - $\lambda_1, MX1, CR1, MN1$ :  
Displays the wavelength at X Cursor 1 and the levels for maxhold, current and minhold.
  - $\lambda_2, MX2, CR2, MN2$ :  
Displays the wavelength at X Cursor 2 and the levels for maxhold, current and minhold.
- $\Delta$ MODE (when MAX HOLD and MIN HOLD are turned off)
  - $\lambda_1, I_1$ : Displays X cursor 1 wavelength, level
  - $\Delta\lambda, \Delta I$ : Displays wavelength difference, level difference between X cursors 1, 2
  - L1,  $\Delta L$ : Displays Y cursor 1 level, level difference between Y cursor 1, 2
- $\Delta$ MODE (when MAX HOLD and MIN HOLD are turned on)
  - $\lambda_1, MM1, MC1, CM1$ :  
Displays the wavelength at X Cursor 1 and the level differences between maxhold and minhold, between maxhold and current, and between current and minhold.
  - $\lambda_2, MM2, MC2, CM2$ :  
Displays the wavelength at X Cursor 2 and the level differences between maxhold and minhold, between maxhold and current, and between current and minhold.
- 2ND PEAK
 

The data display format is as follows. The X cursor 1 automatically moves to the maximum peak and the X cursor 2 to the secondary peak.

  - $\lambda_1, I_1$ : Displays the peak wavelength, level
  - $\Delta\lambda, \Delta I$ : Displays the wavelength difference and level difference between peak and 2nd peak
- POWER
 

X cursor 1 and X cursor 2 automatically move to the maximum peak.

  - $\lambda_1$ : Displays the wavelength at X cursor 1
  - $\lambda_2$ : Displays the wavelength at X cursor 2
  - $\Sigma L$ : Displays the sum of the X cursor 1 and X cursor 2 levels
- PEAK TO PEAK
 

X cursor 1 and X cursor 2 automatically move to the maximum peak and the minimum level data, respectively. Only the peak values are used.

  - $\lambda_1, I_1$ : Displays the wavelength and level at X cursor 1
  - $\lambda_2, I_2$ : Displays the wavelength and level at X cursor 2
  - $\Delta\lambda, \Delta I$ : Displays the wavelength difference and level difference between X cursor 1 and X cursor 2

## 5.7 Setting Limit Line

## 5.7 Setting Limit Line

To set the limit line, load the data file created in the specified format from a floppy disk into the optical spectrum analyzer.

Limit line data files should be created on external personal computers.

## 5.7.1 Data Files

Create data files in text format, and save them in the floppy disk root directory. File names are limited to lmtln1.txt thru lmtln5.txt (the uppercase and lowercase variations are ignored, and the 2-byte character mode cannot be used).

## 5.7.2 Limit Line Data

The limit line data consists of the header block and the data table.

- Header block

The headers below are used to set each item in the header block.

[FUNDAMENTAL]	measmode and domain
[ETC]	warning and label
[REFERENCE]	refmodex, userrefx, offsetx, refmodey, userrefy and offsety
[TABLEUP]	Specifies the upper limit line data.
[TABLELOW]	Specifies the lower limit line data.

Header blocks can be omitted as a general rule. If omitted, the initial values are used (however, either TABLEUP or TABLELOW must be specified).

The details for the above parameters are as follows:

measmode	Specifies a display mode for measurement data (Initial value: measmode=spectrum). Select a display mode from spectrum, peak normalize, loss and trans.
domain	Specifies a unit for the limit line data along the X axis (Initial value: domain=wave) Select a unit from wave (wavelength) and freq (frequency).
warning	Output when the measurement conditions (span) specified for a Pass/Fail judgment is narrower than the range (span) specified for the limit line (Initial value: warning=on). Select on and off.
label	The contents of a label is specified between a pair of double quotations. (The initial label cannot be changed.) Up to the first 48 characters are valid when 49 or more characters are specified.
refmodex	Specifies a description format for the limit line data table (in relative or absolute values). Select it from center, user and abs (Initial value: refmodex=abs).
center	A value (along the X-axis) relative to the specified center wavelength (frequency) is specified in the data table.
user	A value (along the X-axis) relative to the wavelength (frequency) specified by userrefx is specified in the data table.
abs	An absolute value along the X axis is specified in the data table.
userrefx	Specifies the reference wavelength [nm] (frequency [THz]) when refmodex is set to user (Initial value: userrefx=0).
offsetx	Offsets the limit line by the set value along the wavelength [nm] (frequency [THz]) (Initial value: offsetx=0).
refmodey	Specifies a description format for the limit line data table (in relative or absolute values). Select a format from ref, user and abs (Initial value: refmodey=abs).
ref	A value (along the Y-axis) relative to the specified ref level (or Display TOP

	Level if set to LOSS/TRANS) is specified in the data table.
user	A value (along the X-axis) relative to the level specified by userrefy is specified in the data table.
abs	An absolute value along the Y-axis is specified in the data table.
userrefy	Specifies the reference level [dB or dBm] when refmodey is set to user (Initial value: userrefy=0).
offsety	Offsets the limit line by the specified level [dB or dBm] along the Y-axis (Initial value: offsety=0).

- Limit line data

There are two types of limit lines: upper and lower limit lines.

The upper limit is defined by the [TABLEUP] header; and the lower limit, by the [TABLELOW] header (only one of them can be used).

Each data on each line represents a point on the measurement screen.

A limit line consists of lines which connect adjacent points.

Points, which consist of a wavelength (frequency) and a level, are delimited with a single comma (without a unit). Each points starts a new line (up to 1024 points can be specified for each line).

The units available for use are 0.001 [nm], 0.0001 [THz], 0.01 [dB] and 0.01 [dBm]. Always arrange points in ascending order of the X-axis. However, never arrange the points in the opposite direction to the X-axis, (thus resulting in returning the points to the origin) because this mode of arrangement is prohibited.

- Sample file

[FUNDAMENTAL]	'Header used to specify the display mode of a limit line.
measmode=trans	'Sets the display mode to the transmission characteristic measurement mode.
domain=wave	'Specifies the unit for the horizontal-axis waveform data.
[ETC]	'Header used to specify the presence or absence of a warning message, or a label.
warning=on	'Warns that the measurement range is narrower than that of the limit lines.
label="FILTER A"	'Enters a label.
[REFERENCE]	'Header used to specify the limit lines.
refmodex=user	'Sets limit line data along the X-axis in the user reference mode.
userrefx=1550.0	'Sets the reference wavelength to 1550 nm in the user reference mode.
offsetx=0	'Does not offset the limit line along the X-axis (Can be omitted).
refmodey=abs	'Sets limit line data along the Y axis in the absolute value mode.
userrefy=0.0	'Invalid because the limit line data along the Y axis is set using an absolute value (Can be omitted).
offsety=0	'Does not offset the limit line along the Y-axis (Can be omitted).
[TABLEUP]	'Header used to set the upper limit line. The points on the limit line are specified with X (wavelength) and Y (level) as shown below:
-20.0, -15.0	'Specifies the point consisting of a reference wavelength of 1550 nm-20 nm (1530 nm) and a level of -15 dB.
-10.0, -15.0	'Specifies the point consisting of a reference wavelength of 1550 nm-10 nm (1540 nm) and a level of -15 dB.
-5.0, -10.0	'Specifies the point consisting of a reference wavelength of 1550 nm-5 nm (1545 nm) and a level of -10 dB.




5.7 Setting Limit Line


-3.0, -3.0	'Specifies the point consisting of a reference wavelength of 1550 nm-3 nm (1547 nm) and a level of -3 dB.
0.0, 0.0	'Specifies the point consisting of a reference wavelength of 1550 nm-0 nm (1550 nm) and a level of -0 dB.
3.0, -3.0	'Specifies the point consisting of a reference wavelength of 1550 nm+3 nm (1553 nm) and a level of -3 dB.
5.0, -10.0	'Specifies the point consisting of a reference wavelength of 1550 nm+5 nm (1555 nm) and a level of -10 dB.
10.0, -15.0	'Specifies the point consisting of a reference wavelength of 1550 nm+10 nm (1560 nm) and a level of -15 dB.
20.0, -15.0	'Specifies the point consisting of a reference wavelength of 1550 nm+20 nm (1570 nm) and a level of -15 dB.

[TABLELOW] 'Header used to set the lower limit line. A point on a limit line is specified by X (wavelength) and Y (level) as shown below:

-20.0, -35.0	'Specifies the point consisting of a reference wavelength of 1550 nm-20 nm (1530 nm) and a level of -35 dB.
-5.0, -20.0	'Specifies the point consisting of a reference wavelength of 1550 nm-5 nm (1545 nm) and a level of -20 dB.
-3.0, -13.0	'Specifies the point consisting of a reference wavelength of 1550 nm-3 nm (1547 nm) and a level of -13 dB.
0.0, -10.0	'Specifies the point consisting of a reference wavelength of 1550 nm-0 nm (1550 nm) and a level of -10 dB.
3.0, -13.0	'Specifies the point consisting of a reference wavelength of 1550 nm+3 nm (1553 nm) and a level of -13 dB.
5.0, -20.0	'Specifies the point consisting of a reference wavelength of 1550 nm+5 nm (1555 nm) and a level of -20 dB.
20.0, -35.0	'Specifies the point consisting of a reference wavelength of 1550 nm+20 nm (1570 nm) and a level of -35 dB.

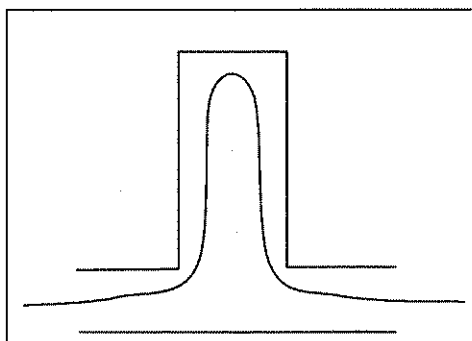


Limit Line Setting Example 1

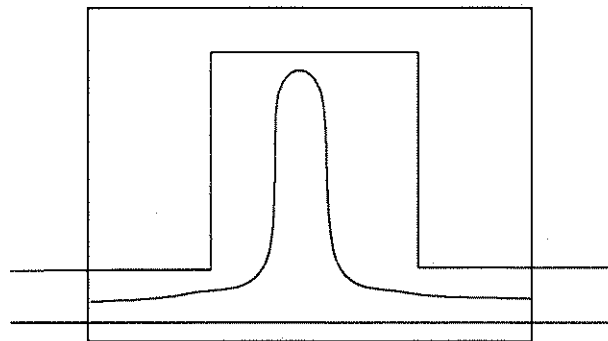


Limit Line Setting Example 2

In Example 1, the measurement range is outside of the limit line range. A PASS/FAIL judgment must always be made within the limit line range, and PASS is displayed in this example.

In Example 2, the limit line range is outside of the measurement range. When Warning is set to on, a warning is issued without making a Pass/Fail judgment. If Warning is set to off, PASS is displayed after a measurement is made within the measurement range.

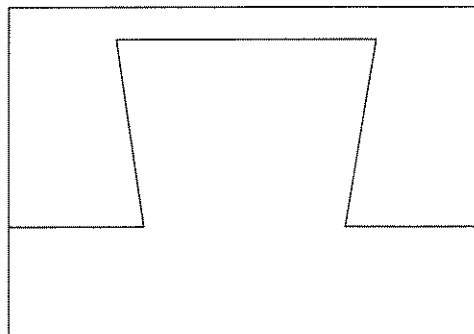

Limit Line Setting Example 3

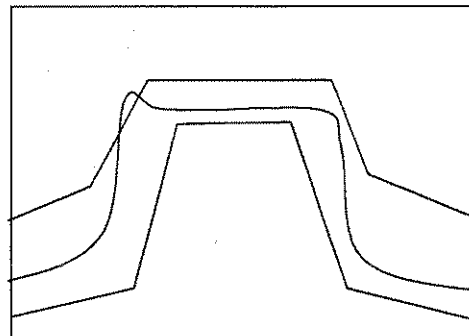

Limit Line Setting Example 4

In Example 3, LIMIT LINE FILE SYNTAX ERROR occurs and nothing will be displayed because the limit line is incorrectly set so that the points return back to the origin along the X-axis.

In Example 4, a part of the waveform is above the upper limit line.

FAIL is displayed after the PASS/FAIL judgment has been made.

5.8 Operation Principle

5.8 Operation Principle

Figure 5-1 is a rough internal block diagram of the optical spectrum analyzer. The analyzer consists of the three blocks: the spectrum (monochromator), measurement control and display processing blocks.

The description below is the operating principle based on this block diagram.

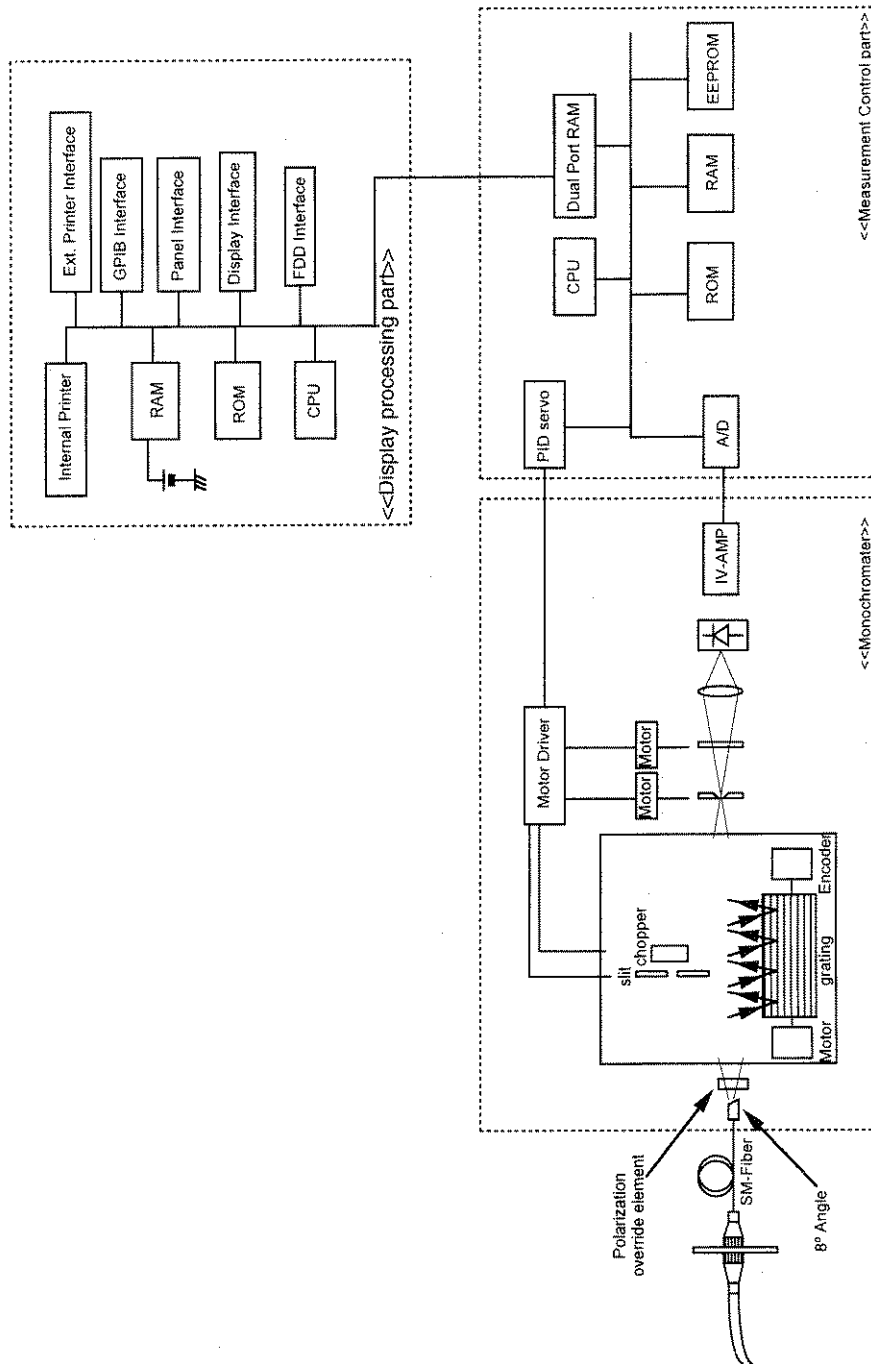


Figure 5-1 Block Diagram

(1) Spectrum block (Monochromator)

In the diffraction grating, there is a spectral characteristic that the angle of the reflecting light is different from the angle of the incident light depending on the wavelength of the incident light. The light to be measured is converted into parallel beam at the collimate mirror and the direction of the reflected light from the diffraction grating differs depending on the wavelength of the light to be measured. This analyzer uses a combination of a diffraction grating and a mirror so that the incident light is diffracted two times to obtain a better resolution. When the rotary angle of the diffraction grating is at a position that matches the incident light wavelength, the diffracted light passes through the converging mirror and the converged light at the mirror passes through the slit, and finally reaches the photodetector. The Q8384 employs the double-path method. Therefore, the light to be measured reaches the photodetector after it passes through the optical system two times. In addition, a special element is used at the monochromator input block to compensate for the polarization dependency (the diffraction efficiency changes depending on the state of the incident light polarization represented by the waves P and S) in order to obtain a constant level regardless of the polarization status.

Sweeping along the wavelengths is performed by rotating the diffraction grating. A high rotational position accuracy is obtained by directly driving the diffraction grating using a servo motor without reduction speed mechanism. In general, the wavelength resolution is determined by the incoming and outgoing slits. The resolution of this analyzer is determined by the intermediate slit typically used in the double-path method because this incoming slit is replaced by the core diameter of the input optical fiber. The intermediate slit has a function of permitting the light with the selected wavelength to be received at the photodetector. The width of the intermediate slit changes according to the set resolution and wavelength. The chopper in front of the intermediate slit chops the light to that it compensates for the offset of the stray light, detector and amplifiers to attain measurements with wide dynamic range. In addition, a light shutter is implemented at the outgoing slit block in order to measure the internal offset generated when the DC amplifier is activated. The photodetector consists of cooling-type InGaAs photodiodes. The light sensed at the photodiodes passes through the current-to-voltage conversion amplifier, range selection amplifier and then reaches the A/D converter. The amplifier block is composed of 11 ranges in increments of 10 dB where an optimum range is automatically selected based on the input signal level. The minimum range for a mode used varies depending on the sweep mode. Furthermore, under control of HI-Dynamic range mode, the signal passes through lock-in amplifiers. When under control of Pulse mode, the signal passes through other dedicated circuit (peak hold circuit).

(2) Measurement control part

This part controls the rotary angle of the diffraction grating, the slit width, and the measurement range, performs the A/D conversion, etc., and transfers the measurement data to the display processing part.

The digital servo circuit by the rotary encode is used for control of the rotary angle of the diffraction grating, allowing high speed, high precision position control.

The stepping motor is used for opening/closing the slit and rotating the chopper, to control the pulse count corresponding to the slit width and to control the pulse period corresponding to the chopper frequency.

Measurement range control includes the auto range control that selects the optimum range, and gate time control when under the pulse mode. The measurement timing (A/D conversion) by the external input signal "GATED MEAS INPUT" is also controlled.

There is also the EEPROM that stores the calibration data (wavelength offset, level offset, wavelength sensitivity offset, etc.) of each monochromator.

## 5.8 Operation Principle

(3) Display processing part

This part controls the measurement system by the conditions set through the panel keys or by the GP-IB, and performs various output processes (display, GP-IB, printer, floppy disk, etc.).

Data exchange with the measurement system is done through the dual-port memory. Measurement conditions as the center wavelength, span, resolution, sweep mode, etc. are sent, while measurement data are received. Wavelength sensitivity offset, display scaling, etc. are performed against the measurement data, and output to the display.

Analysis as cursor processing, spectral width operation, normalization operation, as well as save/recall against the memory/ floppy disk are done.

## 5.9 Notes on Using the Optical Spectrum Analyzer

Pay attention to the items shown below when using the optical spectrum analyzer.

### 5.9.1 Optical Fibers Suitable for the Optical Spectrum Analyzer

Single mode fibers with a mode field diameter of 9  $\mu\text{m}$  to 10  $\mu\text{m}$  are suitable for the optical spectrum analyzer. We recommend that the end face of input fiber be compliant with the super PC specifications and its accuracy be a master A class. If fibers that do not meet these specifications are used, measurements may not be accurate.

### 5.9.2 Stray Light

There is a possibility that a spurious of low level stray light (with a level of 30 to 50 dB below the level at the highest peak and a wavelength of 100 nm to 400 nm away from the highest peak) appears. If the waveform resolution is lowered, the stray light is reduced accordingly. As a result, to decrease the stray light, the wavelength resolution must be raised or the measurement mode must be set to Hi-Dynamic mode.

### 5.9.3 Secondary Diffracted Light

If the incident light wavelength is 633 nm, a secondary diffracted light (with a wavelength of 1266 nm) is usually observable, depending on the diffraction grating characteristics. This is caused by a characteristic of the diffraction grating, and is not a problem.

## 6 SPECIFICATIONS

The following is the specifications of this analyzer.

Characteristics		Specification	
Wavelength	Measurement range	600 nm to 1700 nm	
	Resolution	Setting	10 pm, 20 pm, 50 pm, 100 pm, 200 pm, 500 pm
		Accuracy (*1,*6)	±3% or less/resolution 50 pm (1530 nm to 1610 nm)
	±2% or less/resolution 100 pm or more (1530 nm to 1610 nm)		
	Accuracy	±500 pm or less	
		±200 pm or less (After a calibration using an external light source) (*1)	
		±20 pm (After a calibration using the built-in light source) (1530 nm to 1570 nm) (*1)	
		±40 pm (After a calibration using the built-in light source) (1570 nm to 1610 nm) (*1)	
	Linearity (*1)	±10 pm or less (1530 nm to 1570 nm)	
		±20 pm or less (1570 nm to 1610 nm)	
Repeatability (*1,*4)	±3 pm or less (1530 nm to 1610 nm)		
Level	Measurement range (*2,*3) (input sensitivity)	-87 dBm to +23 dBm (1250 nm to 1610 nm)	
		-77 dBm to +23 dBm (950 nm to 1250 nm, 1610 nm to 1700 nm)	
		-55 dBm to +23 dBm (600 nm to 950 nm)	
	Accuracy (*1,*3)	±0.4 dB or less (1550 nm)	
	Flatness (*1)	±0.2 dB or less (1530 nm to 1610 nm)	
	Repeatability (*1,*3,*4)	±0.02 dB or less (1530 nm to 1610 nm)	
Polarization dependency (*1,*3)	±0.05 dB or less (1250 nm to 1610 nm)		
Level	Dynamic range (*1,*5)	50 dB (±100 pm level difference from peak wavelength)	
		60 dB (±200 pm level difference from peak wavelength)	
		67 dB (±400 pm level difference from peak wavelength, High DR mode)	

6 SPECIFICATIONS

Characteristics		Specification
Sweep	Span	Full span from 0.2 nm and zero span
	Sampling points	101, 201, 501, 1001, 2001, 5001, 10001
	Measurement time	500 msec or less (10 nm span, Normal mode, 1550 nm, 501 points)
Pulse light measurement	Peak hold mode	Minimum light pulse width: 10 ns (Recommended light pulse width: 30 $\mu$ sec or more) Pulse light repetition frequency: 1 Hz or more Gate time: 1ms to 10 s
	External synchronization mode	Synchronization signal input level: 74 AC (Hi:3.5 V, Lo:1.5 V) Synchronization signal pulse width: 10 ns or more.
	Sync Low mode	Synchronization signal (Input): Positive logic Minimum light pulse width: 10 ns (Recommended light pulse width: 30 $\mu$ sec or more)
	Sync Hi mode	Synchronization signal (Input): Leading edge    Sampling time: 0 to 1000 $\mu$ sec
Processing function	Memory function	Internal RAM: Measurement data; 15 or more screens (Sampling points 501, battery backup) Internal FD: 3.5-inch 2HD 1.44 MB with the MS-DOS format
	Display	Horizontal display in wavelengths or frequencies, Superimpose display, Dual Screen display, cursor display and Multi-Trace display (Up to 32 traces)
	Operation/analysis	Auto peak search, auto peak center, auto reference, spectrum analysis (threshold, envelope, RMS, Peak RMS, Xnm level), notch width analysis (XdB width and Xnm level), WDM signal analysis (wavelengths, levels, ITU-T grids and SNRs of up to 256 channel), optical amplifier NF analyzer function (up to 256 channel), normalization using the zooming function (LOSS/TRANS), the peak power monitor function (with trend-chart), and WDM monitor function and limit line function
	Others	Calibration function for the built-in and external light sources, calibration function for wavelength and level offset, and labeling function
Input/ Output	Input connector	FC type (standard), ST type, Sc type (Optional)
	Input Fiber	9.5/125 $\mu$ m SM fiber (Master A grade connector is recommended.)
	Return loss	35 dB
	Data output	GPIB standard, internal/external printer



Characteristics		Specification
General specifications	Operation environment	Temperature +10°C to +40°C, relative humidity 85% or less (no condensation)
	Shelf environment	Temperature -10°C to +50°C, relative humidity 90% or less (no condensation)
	Power supply	100 VAC to 120 VAC or 220 VAC to 240 VAC, 50/60 Hz, 200 VA or less
	External dimension	Approx. 424(W) x 221(H) x 500(D) mm
	Mass	29 kg or less
Optional Built-in EE-LED light source	Center Wavelength	Approx. 1550 nm
	Power (*1)	-45 dBm/nm or more (at 1550 nm)

\*1: With 23°C ± 5°C

\*2: With 10°C to 30°C

\*3: With 100 pm resolution

\*4: 1 minute repeat sweep

\*5: With wavelength 1523 nm (10 pm resolution)

\*6: Calibrated using the effective bandwidth

## APPENDIX

### A.1 Glossary

#### Automatic power control (APC)

The mechanism for supplying power so that the optical output is kept constant. The optical output from a laser diode driven by constant current falls or stops when the temperature rises, and increases when the temperature lowers. The optical output may exceed the maximum rating when the temperature is too low. In order to protect the laser diode and stabilize the optical output, this circuit receives the monitor light of laser diode through the photo diode and then make it feed back to the drive circuit for laser diode.

#### Avalanche photo diode

A light-receiving element frequently used for optical-fiber communications. It uses an avalanche effect: a high reverse bias-voltage (100V to 200V) given to a semiconductor pn junction first moves a few carriers, causing successive carriers to be generated and making the current increase at an accelerated rate.

#### Baseband transmission characteristics

When an optical pulse is input to an optical fiber, the output pulse at the other end diverges, and this phenomenon is called divergence. That is, the transmission loss increases in the time domain. When converted to the frequency domain, it shows an increase in the transmission loss in the high-frequency band. The transmission characteristics in this frequency domain are called the baseband transmission characteristics, and these are important for optical-fiber performance.

#### Beam divergence angle


The angle from the optical axis that halves the radiant intensity from its maximum. For a laser diode, the horizontal direction to the junction is indicated by  $\theta_{//}$  and the perpendicular direction is indicated by  $\theta_{\perp}$ . ( $\theta_{\perp} > \theta_{//}$ )

#### Chopped light

A light with its intensity modulated by a square wave. Its optical output goes on and off repeatedly at a certain cycle.

#### Cladding

A part of the optical-fiber structure. An optical fiber consists of the core axis and the cladding surrounding the core. The fibers are generally made of quartz glass or plastics. The cladding has a refractive index approximately 1% less than that of the core, which helps contain the light flux within the core.

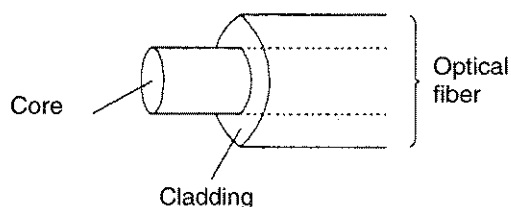

A.1 Glossary

**Coated fiber**

One type of optical fiber, the core and cladding of which are covered by primary coating (silicon resin) and secondary coating (protective nylon layer).

**Coherence**

1. The existence of a timing correlation between the phases of two or more waves.
2. When the wavelengths, phases, and wave faces of light are exactly the same, the light is said to be coherent. There are two types of coherence: temporal and spatial. Temporal coherence is wavelength uniformity and phase continuity. Spatial coherence is the convergence of light into one point by a lens. As represented by laser light, light that has a constant wavelength and stable phase relationships is called coherent.

**Coherent**

Light is one type of electromagnetic wave, and has an extremely short wavelength. However, visible light has characteristics significantly different from those of the electromagnetic waves used for radio and TV programs. That is, while the frequencies, phases, and wave faces of electromagnetic waves are exactly the same, those of visible light vary. Visible light is therefore regarded as a certain type of noise. Light that has exactly the same frequencies, phases, and wave faces is said to be coherent. The light emitted from a laser diode used for optical communications has very high coherence, although it is not perfect.

**Continuous-wave (CW) light**

A non-modulated light with constant intensity. Also known as a DC light.

**Core**

Part of the optical-fiber structure. The core is the central axis, surrounded by cladding. A light flux propagates through the core. It is made of quartz glass and has a refractive index that is larger than that of the cladding by 1%. There are two types of optical fiber: multi mode fibers, with a core thickness of 50 to 100  $\mu\text{m}\phi$ , and single-mode fibers, with a core thickness of approximately 10  $\mu\text{m}\phi$ . Optical fibers can also be classified into the graded index (GI) and step index (SI) types, depending on the refractive index distribution of the core.

**Core and cladding**

The core is the central axis of the optical fiber, and cladding covers the core. Because the cladding has a lower refractive index than that of the core, the incident light propagates through the core, within which it is contained, repeating total reflection at the boundary face between the core and cladding. Generally, the core and cladding diameters are indicated as 50/125  $\mu\text{m}$ , which means a core diameter of 50  $\mu\text{m}$  and a cladding diameter of 125  $\mu\text{m}$ .

**Dark current**

Current output from a light-receiving element when no incident light is given to it.

**Direct modulation**

The method that use a modulating signal as drive current to turn the light source on. The method of using a lightwave modulator is called external modulation.

**Directivity**

The property of having a large optical output or responsivity in a specific direction.

**Distributed feedback laser (DFB-LD)**


A type of laser that has a waveguide with a cyclic structure, to form a resonator that has a selective wavelength.

**Double heterojunction**

A heterojunction means a junction by crystals with different atomic structures. The double heterojunction in laser diodes places a cladding layer with a large energy gap on both sides of the active layer. It is used to raise the minority carrier density and to form an optical waveguide.

**Emission peak wavelength**

The wavelength of a light-emitting element that produces the maximal energy density of the emission spectrum.

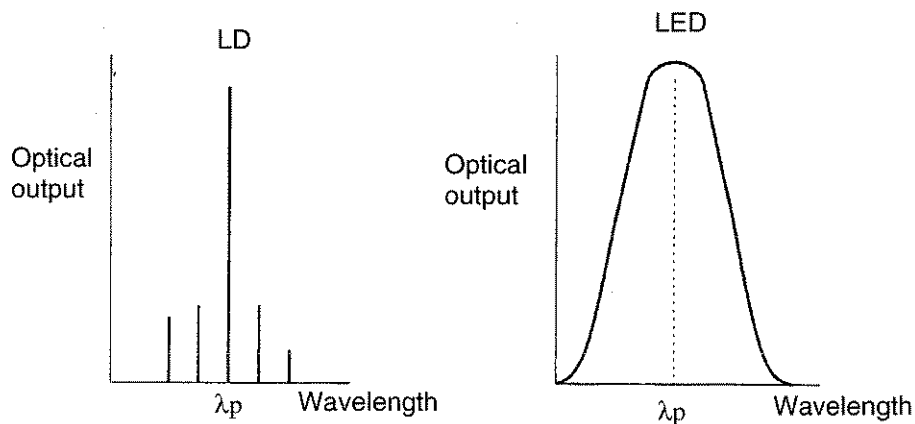**Excess noise factor**

Factor of shot noise multiplication occurring in an avalanche photodiode. It is defined as  $F = Mx$ .

Because of the fluctuation in the multiplication process, shot noise current  $i_N$  increases as

$$\langle i_N^2 \rangle = 2qIM^{2+x} B.$$

M: Multiplication factor

B: Signal bandwidth

x: Excess noise factor

q: Electron charge

I: Average current flowing in the avalanche area

**FM**

Frequency modulation

A.1 Glossary

**Fundamental mode**

0-dimensional electromagnetic field distribution. Also known as single lateral mode.

**Graded index fiber**

One type of multi mode fiber, the core refractive indices of which are distributed in a parabolic form. This means that the light passing through the center of the core goes more slowly, and the light passing through the periphery goes faster, making the propagation speed constant regardless of the light path. In addition, the timing distribution of output pulses can be made extremely small (little mode dispersion). This means that the transmission band (hundreds of MHz · km) is much wider than that of the step index fiber.

**IM**

Intensity modulation

**Infrared rays**

Light with wavelengths longer than those of visible light.

Wavelength 0.78 to 3 μm: Near-infrared light

3 to 30 μm: Mid-infrared light

30 μm to 1 mm: Far-infrared light

1mm or more: Microwave

**Laser**

There are several types of laser: solid-state, gas, liquid, etc. Solid-state lasers are used as the light source for optical-fiber communications, because they are smaller than other types of laser and allow direct modulation. Compared to LEDs, lasers have better coherence and faster responses, and they are therefore important elements as a light source. A solid-state laser is sometimes abbreviated LD, standing for laser diode.

**Laser diode**

One type of semiconductor light-emitting element. The word laser stands for Light Amplification by Stimulated Emission of Radiation. A laser is an oscillator that emits light using this principle. A laser diode gives a high optical output. Laser diodes have advantages such as high optical output, the possibility of fast direct modulation, good optical-fiber coupling efficiency, etc., but they have a problem in the stability of the light emission. This is why LEDs have mainly been used. Recently, since this problem is now being solved, laser diodes are being used more than before for long-distance, fast communications.

**Leak light**

When an optical fiber is bent or pressed, the light propagation path in the core is distorted, causing the propagating light to leak out of the optical fiber. This is called leak light.

**Light-emitting diode (LED)**

One type of light-emitting element. As in the case of a laser diode, it uses the light emitted when the carriers injected into the semiconductor pn junction face recombine. In a laser diode, light is generated by induced emission, whereas in an LED it is generated by spontaneous emission. An LED has advantages such as long life, stability, low cost, and good linearity. However, because an LED produces only a small output to send to the fiber and is not suitable for fast modulation, it is advantageous for short-distance, small-capacity communications or analog-type communications.

**Light sensor**

For optical-fiber communications, a photodiode (PD) using the photovoltaic effect or photoconductive effect is used. There are two types of PDs: pn and pin. Those applying the avalanche effect by giving reverse bias voltage are called avalanche photodiodes (APD). These photoreceivers are mainly used for measurement devices. In addition, thermopiles employing the thermo effect have constant sensitivity regardless of the wavelength, and are used as detectors in reference optical power meters.

**Longitudinal mode**

A state which emission spectrum, that a half height width is extremely small, exist discontinuously. An individual emission spectrum is also called a longitudinal mode. The wavelength difference with the adjacent mode is called a longitudinal mode interval. When there is only one mode, it is called a single longitudinal mode.

**Long wavelength region**

Among the optical wavelengths used for optical-fiber communications, this is the region of 1.0 to 1.5  $\mu\text{m}$ . This region is used for long-distance communications, because it produces little transmission loss with optical fibers.

**Luminous flux**

$$F = K_m \int_{380}^{780} V(\lambda) d\lambda$$

Unit: lm (lumen)

$K_m$ : Maximum visibility 680lm/W

$V(\lambda)$ : Standard spectral luminous efficiency

Value determined by International Commission on Illumination (CIE)

1.0004 when  $\lambda = 555\text{nm}$  (yellow-green)

**Luminous intensity**

$$i = \frac{dF}{dw}$$

Unit: Cd (candela)

$F$ : Luminous flux

$w$ : Solid angle

Radiant intensity is the value indicated by an energy unit.

### Mach-Zehnder interferometer

A type of interferometer which the incident light is split into two routes, and a delay is given to one route but not to the other. The two waves are then composed again to cause interference.

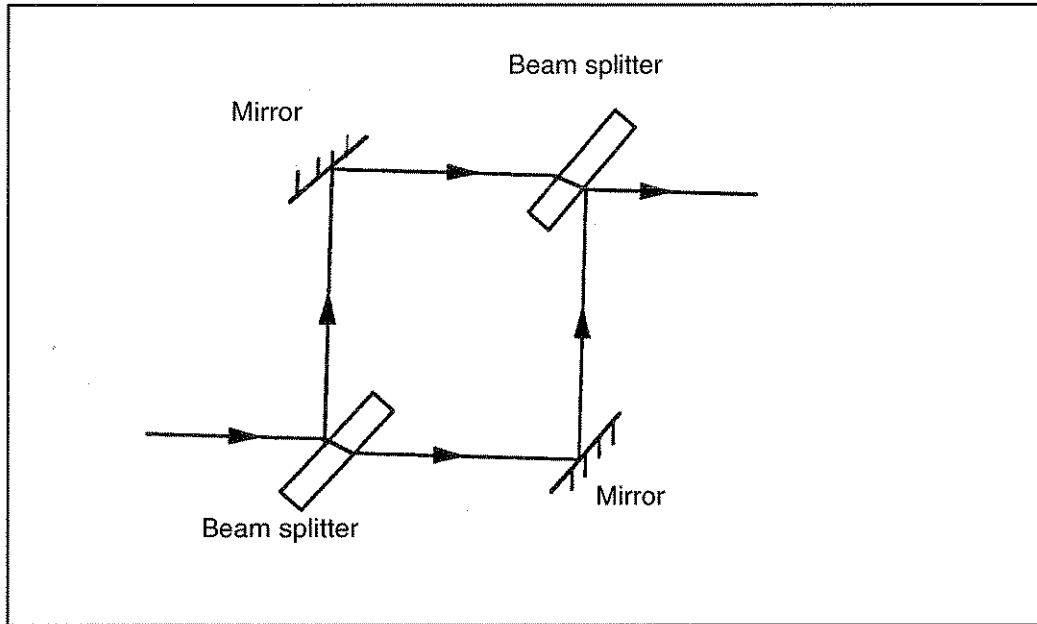


Figure A-1 Typical Mach-Zehnder Interferometer Configuration

### Monitor current

Monitor diode output generated when the light emitted from the rear of the laser diode chip is received by the monitor diode.

### Monitor output

A light emitted from the rear of the laser diode chip.

### Multi mode fiber

An optical fiber that has more than one propagation mode, and many of these modes (which can be assumed to be light with various angles to the optical fiber's central axis) propagate through the core at the same time. Multi mode fibers can be classified into step, graded, and other types, depending on the refractive indices of the core. They are advantageous in that the core diameter is comparatively large (50 to 100  $\mu\text{m}$ ), and connections are easier than with single mode fibers. On the other hand, the transmission band area is somewhat narrow (mode divergence), because many modes propagate at different speeds through the optical fiber.

**Numerical aperture**

The degree of extension of light at the end of an optical fiber, which has a cylindrical core having a refractive index of  $n_1$  and which is surrounded by clad having a refractive index of  $n_2$  ( $n_1 > n_2$ ), due to a similarity in the lens system. Of the light falling on a plane, which includes the axis of the core of the optical fiber and which crosses the axis (the meridian light), if some light, which attains critical angle with respect to the axis, crosses the axis of the core outside the optical fiber at angle  $\theta$ , the NA of the optical fiber can be expressed by the equation given below.

$$NA = n \sin \theta = \sqrt{n_1^2 - n_2^2}$$

$n$ : Refractive index of the media in which the optical fiber is placed

**Optical fiber**

An optical waveguide in which the outer refractive index is made less than the inner one to give the fiber such characteristics that enable the light to propagate inside the fiber, even when the fiber is bent.

A fiber with a diameter of approximately 0.12mm $\phi$  consisting of two types of quartz glass (core and cladding) with different refractive indices. It shows superior characteristics such as wide band, small loss, and noninduction.

**Optical fiber connector**

A detachable connector for connecting optical fibers to one other, or an optical fiber to a device. Usually simple matching is used for connection, that is, optical-fiber faces are connected directly to each other by using connectors with their cores well aligned. Compared with electrical connectors, an optical fiber connector has some disadvantages: high mechanical precision is necessary, a connection loss of approximately 0.5 to 1dB occurs, and careful treatment is required to prevent dust.

**Optical rotating power**

A phenomenon in which the plane of polarization rotates when a linear polarized light passes through a substance.

**Pigtail fiber**

A fiber with its one or both ends are open.

**Polarizer**

An element that converts natural light into a linear polarized wave.



A.1 Glossary

**Quantum efficiency**

- Light-emitting element (light-emitting diode, laser diode)

The ratio of the number of photons generated inside an element to the number of carriers generated (internal quantum efficiency); or the ratio of the number of photons emitted outside to the number of generated carriers (external quantum efficiency).

The quantum efficiency can be expressed as follows:

$$\eta = \frac{q\lambda}{hc} \cdot \frac{p}{I} = \frac{\lambda}{1.24} \cdot \frac{p}{I}$$

h: Planck's constant

c: Light speed in vacuum

q: Charge of electron

$\lambda$ : Wavelength ( $\mu\text{m}$ )

P: Optical output

I: Current

In addition, a differential quantum efficiency is also used for a laser diode.

- Light receiving element (PIN photodiode APD)

The ratio of the number of generated carriers to the number of input photons. The quantum efficiency  $\eta'$  is expressed as follows. This is the reverse of that of a light-emitting diode

$$\eta' = \frac{hc}{q\lambda} \cdot \frac{I}{P} = \frac{1.24}{\lambda} \cdot \frac{I}{P}$$

The quantum efficiency of an avalanche photodiode is calculated assuming that the multiplication factor is 1.

**Radiant flux**

Optical energy emitted and propagated in a unit of time.

**Responsivity**

Current that can be generated when a unit radiant flux is input to a light-receiving element.

$$R = \frac{I}{P} = 0.806 \times \eta \times \lambda \times M \text{ [A/W]}$$

R: Responsivity

$\eta$ : Quantum efficiency

$\lambda$ : Wavelength

M: Multiplication factor

**ROM**

Stands for Read-Only Memory.

**Short wavelength region**

Optical-fiber communications use light with a wavelength of approximately 0.8 to 1.5  $\mu\text{m}$ , or the near-infrared region. Within this region, the region around 0.8  $\mu\text{m}$  is called the short-wavelength region. This region was developed during an earlier stage in the field of optical-fiber communications, and produced the largest number of results for production systems. Recently, the long wavelength region exceeding 1  $\mu\text{m}$  has been under development.

**Single-mode fiber**

When the core diameter is reduced to approximately 10  $\mu\text{m}$ , the result is an optical fiber with only one propagation mode. This is called a single-mode fiber. This fiber is advantageous in that, unlike the multi mode fiber which causes mode distribution, it has a very wide range (a few GHz).

**Specific rotating power**

A value indicating the magnitude of the optical rotary power of material.

**Speckle effect**

A noise generated when a coherent light is dispersed in an optical fiber, causing interference under irregular phase relationships.

**Spectral width/Full width at half maximum/ $\Delta\lambda$** 

An interval between two wavelengths of a light emitting element, in which the emission spectrum energy is half the maximal value.

**Spectrum**

An ordinary light consists of sine wave components. An array of such components arranged along the wavelength axis is called a spectrum.

A white light source has a flat spectrum, and an LD has one concentrated in a narrow area.


**Splicing**

Permanent connection of an optical fiber, necessary for optical-fiber cabling operations. Although there are various splicing methods, the method generally used is fusion splicing, in which glass is melted by arc discharge. This method allows stable connections with the least connection loss.

A.1 Glossary

**Threshold current**

Minimum current that allows laser emission. Since the boundary area between the spontaneous and laser emissions is not rigid, it is sometimes represented by the crossing point of the line prolonged from the current optical output characteristics curve for laser oscillation and the current value for optical output zero.

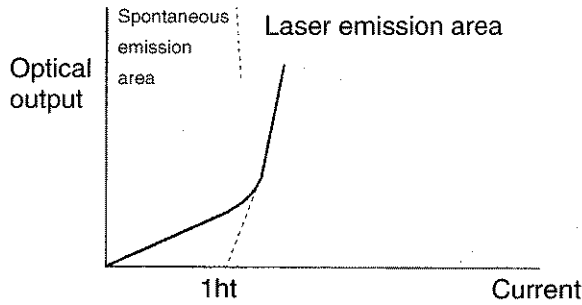

**Ultraviolet rays**

Light with a shorter wavelength than visible light. The wavelengths range from 300 to 380nm.

**Visible light**

Light that can be seen by the human eye. The wavelength range is 380 to 780nm.

**Wavelength division multiplying**

A communication method in which two or more types of signals are simultaneously transmitted through one optical fiber. In the transmitter, light-emitting and laser diodes of various wavelengths are used. This method allows one-way or two-way communications.





## A.2 Error Messages

Message	Description
LIGHT POWER IS TOO LOW	The light source power level of the used for calibration or alignment is too low.
LIGHT SOURCE ERROR	The light source used for calibration is inappropriate.
TOO LARGE ERROR	The light source wavelength used for calibration or alignment is very different from the specified value.
DISK FORMATTING FAILED	The floppy disk cannot be formatted.
FLOPPY MEDIA TYPE[2DD/2HD] ERROR	When formatting, a wrong floppy disk is inserted.
DISK FULL	There is no disk space to create a new file.
MEMORY FULL	There is no disk space to create a new file in the internal data memory.
DISK READ ERROR	Cannot read data from the disk correctly.
DISK WRITE ERROR	Cannot write data on the disk correctly.
ILLEGAL FILE NAME	When writing data, an illegal file name was assigned.
INTERVAL TIME IS TOO SHORT	Warning issued when the actual measurement could not be completed within the measurement interval set prior to starting the peak power monitor or WDM monitor.
MEDIA NOT IN DRIVE	No disk is inserted in the drive.
TOO MANY FILES TO WRITE	The number of files exceeds the maximum value.
PRINTER ERROR (EXT. PRT)	Abnormal conditions are detected in the external printer cable, or the printer is out of paper.
NO PRINTER PAPER (INT. PRT)	The built-in printer runs out of paper.
PRINTER HEAD UP (EXT. PRT)	The printer head is in the raised position.
PRINTER IS NOT READY	The external printer cannot print.
PRINTER NOT RESPONDING	The external printer does not respond to commands.
LIMIT FILE NOT FOUND	No limit line data was found in the floppy disk.
PATTERN X NOT LOADED	The specified limit line data has not been loaded into memory.
DIFFERENT MEAS MODE	The mode for the limit line data does not match the current measurement mode.
LIMIT LINE NOT DISPLAY	A Pass/Fail judgment was attempted when no lines were being displayed.
LIMIT LINE EXCEEDS MESUREMENT AREA	The limit line set while Warning was turned on was outside of the measurement range.
LIMIT LINE SYNTAX ERROR	Syntax error in the limit line error



Items have the following meanings.

- (1) Manufacturer, model name, software version and type of analysis data
  - (2) Label and time
  - (3) Center wavelength [m], span wavelength [m], start wavelength [m] and stop wavelength [m]
  - (4) Number of point averages, number of sweep averages, number of smoothing processes, REF LEVEL, vertical scale, Linear/Log ON/OFF
  - (5) Frequency mode ON/OFF, number of sampling processes, wavelength resolution, measurement mode, MAX HOLD ON/OFF, MIN HOLD ON/OFF, PM ON/OFF (peak power monitor)
  - (6)  $\lambda$  offset and level offset
  - (7) PM N-MAX, PM interval, PM wavelength, PM minimum, PM maximum and PM average
  - (8) Empty
  - (9) Displaying the measurement data
  - (10) Measurement data [nm], [dBm]
- \* When the horizontal axis is set to the frequency mode, FRQ is 1 and items (3) and (10) are as follows:  
For (3), center frequency [Hz], span frequency [Hz], start frequency [Hz] and stop frequency [Hz].  
For (10), Measurement data [THz], [dBm]
- \* When the vertical axis is set to the linear, LIN is 1 and item (10) (measurement data power level) is changed to a power level [mW].

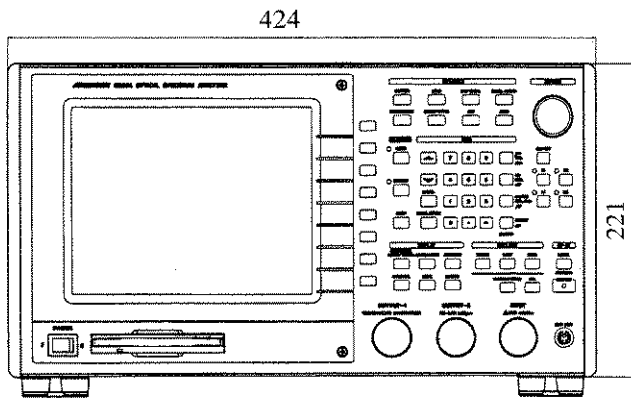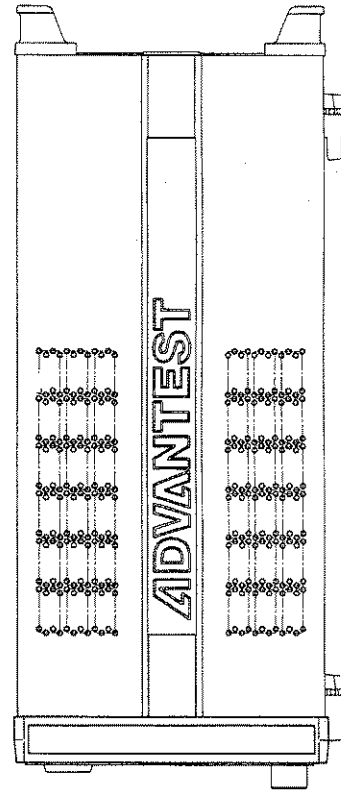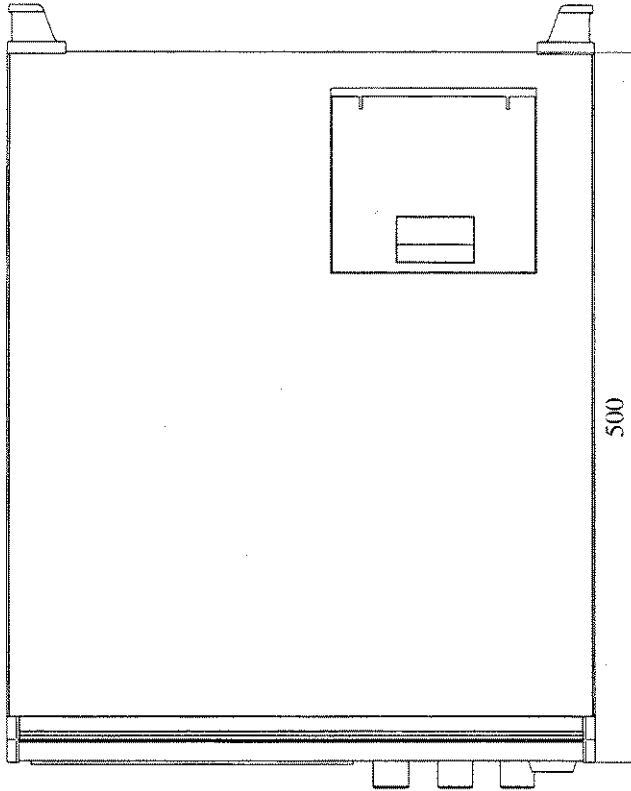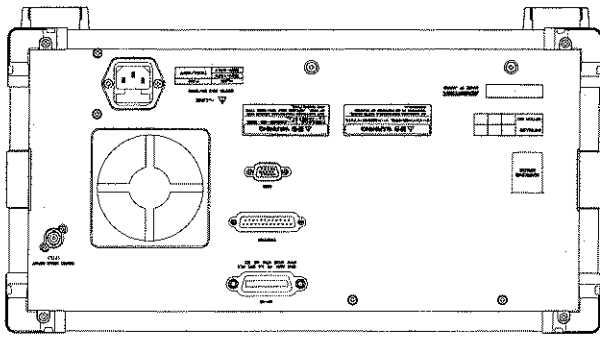

424

Unit : mm

**CAUTION**

This drawing shows external dimensions of this instrument.  
The difference in products and options used can cause a change in the appearance of the instrument.

**DIMENSIONAL OUTLINE DRAWING**

## ALPHABETICAL INDEX

	<b>[Symbol]</b>			
$\Delta$ MODE	.....	3-10, 3-34	3	..... 3-6, 3-22
$\lambda$ drift Lmt.	.....	3-9, 3-32	3.5-inch floppy disk	..... 1-2
$\lambda$ OFFSET	.....	3-14, 3-43	32	..... 3-6, 3-22
$\lambda.f$	.....	3-9, 3-29	4	..... 3-6, 3-22
$\lambda_1$	.....	3-10	5	..... 3-6, 3-22
$\lambda_1$ Key	.....	3-34	5001	..... 3-11, 3-36
$\lambda_2$	.....	3-10	501	..... 3-11, 3-36
$\lambda_2$ Key	.....	3-34	5dB/D	..... 3-5, 3-18
→	.....	3-8, 3-9, 3-12, 3-14, 3-26, 3-28, 3-30, 3-37, 3-44	64	..... 3-6, 3-22
←	.....	3-8, 3-9, 3-12, 3-14, 3-26, 3-28, 3-30, 3-37, 3-44	7	..... 3-6, 3-23
↑	.....	3-8, 3-9, 3-26, 3-28, 3-30	8	..... 3-6, 3-22
↓	.....	3-8, 3-9, 3-26, 3-28, 3-30	9	..... 3-6, 3-23
	<b>[Numerics]</b>			
0.01nm	.....	3-6, 3-19		
0.02nm	.....	3-6, 3-19		
0.05nm	.....	3-6, 3-19		
0.1dB/D	.....	3-5, 3-18		
0.1nm	.....	3-6, 3-19		
0.2dB/D	.....	3-5, 3-18		
0.2nm	.....	3-6, 3-19		
0.5dB/D	.....	3-5, 3-18		
0.5nm	.....	3-6, 3-19		
1(OFF)	.....	3-6, 3-22		
10001	.....	3-11, 3-36		
1001	.....	3-11, 3-36		
101	.....	3-11, 3-36		
10dB/D	.....	3-5, 3-18		
11	.....	3-6, 3-23		
16	.....	3-6, 3-22		
1dB/D	.....	3-5, 3-18		
2	.....	3-6, 3-22		
2001	.....	3-11, 3-36		
201	.....	3-11, 3-36		
2dB/D	.....	3-5, 3-18		
2DD(720K)	.....	3-13, 3-40		
2HD(1.44M)	.....	3-13, 3-40		
2ND PEAK	.....	3-10, 3-34		
			<b>[A]</b>	
			ABORT	..... 3-7, 3-23
			ABSOLUTE	..... 3-9, 3-30
			absolute/relative	..... 3-9, 3-30
			Accessories	..... 1-2
			ACT U&L ON/OFF	..... 3-11, 3-35
			ADAPTIVE	..... 3-6, 3-20
			ADDRESS DOWN	..... 3-14, 3-42
			ADDRESS UP	..... 3-14, 3-42
			ADVANCE	..... 3-10
			ADVANCE Key	..... 3-33
			Alignment	..... 2-24
			APC	..... A-1
			APPLICATION	..... 3-8
			APPLICATION Key	..... 3-25
			ASE Converted NBW	..... 3-8, 3-9, 3-29, 3-32
			ASE Fitting	..... 3-8, 3-9, 3-27, 3-28, 3-31
			ASE NBW	..... 3-8, 3-9, 3-29, 3-31
			AUTO	..... 3-7
			AUTO ALIGNMENT	..... 3-14, 3-43
			AUTO Key	..... 3-23
			AUTO ON/OFF	..... 3-11, 3-36
			AUTO PKC ON/OFF	..... 3-5, 3-15
			AUTO RELV ON/OFF	..... 3-5, 3-17
			AUTO TRAC ON/OFF	..... 3-11, 3-35
			Automatic power control	..... A-1
			Auto-Panning and Auto-Zooming	
			Functions	..... 5-12
			Avalanche photo diode	..... A-1
			Averaging Functions	..... 5-2
			AVG	..... 3-6
			AVG Key	..... 3-22



Alphabetical Index

**[B]**

Backup Memory ..... 2-60  
 Baseband transmission characteristics .... A-1  
 Basic Operation ..... 2-12  
 Beam divergence angle ..... A-1  
 BEEP ON/OFF ..... 3-13, 3-41  
 bit map ..... 3-13, 3-40  
 buzzer ..... 3-13, 3-41

**[C]**

CAL ..... 3-14  
 CAL Key ..... 3-43  
 CAL  $\lambda$  (Ext.) ..... 3-14, 3-43  
 CAL  $\lambda$  (Int.) ..... 3-14, 3-43  
 Calculating the Half-height Width and  
 the Notch Width ..... 5-3  
 Calibration ..... 1-12, 2-26  
 CENTER ..... 3-5  
 CENTER Key ..... 3-15  
 Chopped light ..... A-1  
 Cladding ..... A-1  
 Cleaning ..... 1-10  
 Cleaning, Storing and Transporting the  
 Q8384 Optical Spectrum Analyzer ..... 1-10  
 CLEAR LINE ..... 3-14, 3-44  
 clock ..... 3-13, 3-40  
 CLOSE ..... 3-8, 3-9,  
 3-26, 3-28  
 Coated fiber ..... A-2  
 Coherence ..... A-2  
 Coherent ..... A-2  
 color ..... 3-13, 3-40  
 COMMAND:ESC/P ..... 3-13, 3-39  
 COMMAND:ESC/P RAS ..... 3-13, 3-39  
 COMMAND:HP PCL ..... 3-13, 3-39  
 COMPRESS ON/OFF ..... 3-13, 3-40  
 Connector Section ..... 2-8  
 Continuous-wave (CW) light ..... A-2  
 CONTROL ..... 3-11  
 CONTROL Key ..... 3-35  
 COPY ..... 3-14  
 COPY Key ..... 3-42  
 Core ..... A-2  
 CURRENT SELECT ..... 3-9, 3-32  
 Cursor Modes ..... 5-13  
 CURSOR Section ..... 2-4  
 CURSOR SPAN ..... 3-5, 3-16  
 CURSOR→CENTER ..... 3-5, 3-15  
 CURSOR→REF LEVEL ..... 3-5, 3-17

**[D]**

Dark current ..... A-2

data mode ..... 3-9, 3-29  
 DATA OUT Section ..... 2-7  
 DATA Section ..... 2-5  
 DAY ..... 3-13, 3-41  
 Defaults Configuration Values ..... 3-45  
 DELAY ..... 3-6, 3-20  
 DELETE ..... 3-12, 3-37  
 DELETE ALL ..... 3-11, 3-35  
 DELETE CHAR ..... 3-14, 3-44  
 DELETE CURRENT ..... 3-11, 3-35  
 DEVICE ..... 3-13  
 Device Clear Function ..... 4-26  
 DEVICE Key ..... 3-39  
 Device Triggering Function ..... 4-26  
 DFB-LD ..... A-3  
 Direct modulation ..... A-2  
 Directivity ..... A-3  
 DIRECTORY ..... 3-13, 3-39  
 DISPLAY MONI/SPEC ..... 3-9, 3-29  
 DISPLAY ON/OFF ..... 3-13, 3-40  
 DISPLAY Section ..... 2-6  
 Distributed feedback laser ..... A-3  
 Double heterojunction ..... A-3  
 DUAL ON/OFF ..... 3-11, 3-35

**[E]**

EDGE RISE/FALL ..... 3-6, 3-21  
 Emission peak wavelength ..... A-3  
 ENTER ..... 3-12, 3-14,  
 3-37, 3-44  
 Entering Label Data ..... 2-57  
 ENVELOPE ..... 3-8, 3-25,  
 5-4  
 Environmental Conditions ..... 1-4  
 Example Programs ..... 4-41  
 Excess noise factor ..... A-3  
 EXECUTE ..... 3-13, 3-14,  
 3-39, 3-43  
 EXIT ..... 3-12, 3-37,  
 3-38  
 EXT KEY US/JP ..... 3-13, 3-40  
 EXTERNAL PRINTER ..... 3-13, 3-39  
 external printer ..... 3-13, 3-39

**[F]**

Fan filter ..... 1-2  
 FC connector ..... 1-2  
 FEED ..... 3-14  
 FEED Key ..... 3-42  
 Filter  $\Delta\lambda$  ..... 3-8, 3-27  
 Fitting Span ..... 3-8, 3-9,  
 3-27, 3-28

Fitting span ..... 3-31  
 floppy ..... 3-13, 3-39  
 FLOPPY DISK ..... 3-13, 3-39  
 Floppy Disk ..... 2-59  
 FM ..... A-3  
 format ..... 3-13, 3-39  
 Front Panel ..... 2-1  
 FULL SPAN ..... 3-5, 3-16  
 FUNCTION Section ..... 2-3  
 Functional Description ..... 3-15  
 Fundamental mode ..... A-4

**[G]**

GAIN ..... 5-9  
 GAIN&NF ..... 5-8  
 GATE TIME ..... 3-6, 3-21  
 Glossary ..... A-1  
 GPIB Command Codes ..... 4-29  
 GPIB Command Index ..... 4-1  
 GP-IB Section ..... 2-7  
 Graph All Data ..... 3-9, 3-30  
 GRAPH X TIME/CH ..... 3-9, 3-29  
 GRID CH Spacing ..... 3-8, 3-9,  
 3-29, 3-32  
 GRID ON/OFF ..... 3-11, 3-35  
 GRID ref. Frequency ..... 3-8, 3-9,  
 3-29, 3-32

**[H]**

Hard Copy ..... 2-62  
 HEADER ON/OFF ..... 3-14, 3-42  
 HI DYNAMIC1 ..... 3-6, 3-20  
 HI DYNAMIC2 ..... 3-6, 3-20  
 HI-SENS1 ..... 3-6, 3-20  
 HI-SENS2 ..... 3-6, 3-20  
 HOUR ..... 3-13, 3-41

**[I]**

INITIAL ..... 3-9, 3-30  
 INSERT SPACE ..... 3-14, 3-44  
 INSTR PRESET ..... 3-14  
 INSTR PRESET Key ..... 3-42  
 Interface Functions ..... 4-4  
 INTERNAL PRINTER ..... 3-13, 3-39  
 INTERVAL TIME ..... 3-10, 3-33  
 INTRODUCTION ..... 1-1  
 ITU GRID ..... 3-8, 3-28

**[K]**

K ..... 3-8, 3-25  
 Kr(RMS) ..... 3-8, 3-25

**[L]**

L1 ..... 3-10  
 L1 Key ..... 3-34  
 L2 ..... 3-10  
 L2 Key ..... 3-34  
 LABEL ..... 3-14  
 LABEL Key ..... 3-44  
 LCD Display Section ..... 2-2  
 LEFT PEAK ..... 3-10, 3-34  
 LEVEL ..... 3-8, 3-9,  
 3-26, 3-30  
 Level Lower Lmt. .... 3-9, 3-31  
 LEVEL OFFSET ..... 3-14, 3-43  
 LEVEL SCALE ..... 3-5  
 LEVEL SCALE Key ..... 3-18  
 Level Upper Lmt. .... 3-9, 3-31  
 Light amplifier Characteristic Analysis .. 2-33  
 Light source used for calibration ..... 1-2  
 Light Spectrum Measurement ..... 2-14  
 limit line ..... 3-10, 3-33  
 Limit Line Data ..... 5-14  
 Limited-life Part ..... 1-2  
 LIST ALL ON/OFF ..... 3-8, 3-29  
 List of Settings ..... 3-45  
 LOAD PATTERN FILES ..... 3-10, 3-33  
 LOCAL ..... 3-14  
 LOCAL Key ..... 3-42  
 LOSS ..... 3-7, 3-24  
 LVL SCALE LIN/LOG ..... 3-5, 3-18

**[M]**

Manual ASE Level ..... 3-8, 3-9,  
 3-27, 3-29,  
 3-32  
 Masked Span ..... 3-8, 3-9,  
 3-27, 3-28,  
 3-31  
 MAX HOLD ON/OFF ..... 3-5, 3-17  
 MAX HOLD→CURRENT ..... 3-5, 3-17  
 MEASURE Section ..... 2-4  
 Measurement Modes ..... 5-1  
 Measurement Times ..... 3-9, 3-31  
 Measuring the Transmission-wavelength  
 (or Loss-wavelength) Characteristics .... 2-29  
 Menu Index ..... 3-1  
 Menu Map ..... 3-5  
 MENU OUT ON/OFF ..... 3-13, 3-39  
 Method ..... 3-8, 3-27  
 MIN ..... 3-17  
 MIN HOLD ON/OFF ..... 3-5, 3-17  
 MIN HOLD→CURRENT ..... 3-5, 3-17  
 MINUTE ..... 3-13, 3-41

## Alphabetical Index

MODE SNG/WDM ..... 3-8, 3-26  
 MODE:COLOR ..... 3-13, 3-40  
 MODE:GRAY ..... 3-13, 3-39,  
 3-40  
 MODE:MONO ..... 3-13, 3-40  
 MODE:MONO L ..... 3-13, 3-39  
 MODE:MONO S ..... 3-13, 3-39  
 MONTH ..... 3-13, 3-40  
 MULTI PEAK ..... 3-8, 3-28  
 multi trace ..... 3-11, 3-35

**[N]**

name ..... 3-12, 3-37  
 NAME CLEAR ..... 3-12, 3-37  
 NEXT ..... 3-11, 3-35  
 NEXT PAGE ..... 3-27  
 NF ..... 5-10  
 NF K ..... 3-8, 3-27  
 NF Select ..... 3-8, 3-26  
 NOMINAL ..... 3-9, 3-30  
 Nominal Level ..... 3-9, 3-32  
 Nominal SNR ..... 3-9, 3-32  
 NORMAL ..... 3-6, 3-10,  
 3-20, 3-34  
 NORMALIZE LOSS/TRANS ..... 3-7  
 NORMALIZE LOSS/TRANS Key ..... 3-24  
 Notch Width ..... 5-6  
 notch width ..... 3-8, 3-26  
 Notes on Using the Optical Spectrum  
 Analyzer ..... 5-21

**[O]**

OFF ..... 3-8, 3-9,  
 3-10, 3-11,  
 3-25, 3-26,  
 3-28, 3-29,  
 3-32, 3-33,  
 3-35  
 ON/OFF ..... 3-10  
 ON/OFF Key ..... 3-34  
 Operating Environment ..... 1-4  
 Operating Menus and Entering Data ..... 2-12  
 OPERATION ..... 2-1  
 Operation Principle ..... 5-18  
 opt.amp ..... 3-8, 3-26  
 Optical Fibers Suitable for the optical  
 spectrum analyzer ..... 5-21  
 Option ..... 1-2  
 Outputting Data ..... 2-62  
 Overview of GPIB ..... 4-3

**[P]**

Panel Description ..... 2-1  
 parameter ..... 3-6, 3-8,  
 3-9, 3-20,  
 3-25, 3-26,  
 3-28, 3-30  
 PASS/FAIL ..... 3-10, 3-33  
 Pass/Fail enable ..... 3-9, 3-31  
 PATTERN-1 ..... 3-13, 3-40  
 PATTERN1 ..... 3-10, 3-33  
 PATTERN-2 ..... 3-13, 3-40  
 PATTERN2 ..... 3-10, 3-33  
 PATTERN-3 ..... 3-13, 3-40  
 PATTERN3 ..... 3-10, 3-33  
 PATTERN-4 ..... 3-13, 3-40  
 PATTERN4 ..... 3-10, 3-33  
 PATTERN-5 ..... 3-13, 3-40  
 PATTERN5 ..... 3-10, 3-33  
 PEAK NORMALIZE ..... 3-7, 3-24  
 Peak Power Monitor Measurement ..... 2-21  
 peak power-mon ..... 3-10, 3-33  
 PEAK RMS ..... 3-8, 3-25  
 Peak RMS ..... 5-5  
 PEAK THRESHOLD ..... 5-3  
 PEAK TO PEAK ..... 3-10, 3-34  
 PEAK→CENTER ..... 3-5, 3-15  
 PEAK→REF LEVEL ..... 3-5, 3-17  
 PEAK-THRESHOLD ..... 3-8, 3-25  
 Pin LOSS ..... 3-8, 3-27  
 point average ..... 3-6, 3-22  
 Pout LOSS ..... 3-8, 3-27  
 POWER ..... 3-10, 3-34  
 Power Cable ..... 1-7  
 Power cable ..... 1-2  
 Power Fuse ..... 1-6  
 Power fuse ..... 1-2  
 Power Monitor Measurement ..... 2-22  
 Power Requirements ..... 1-5  
 POWER Switch/Floppy Disk Drive  
 Section ..... 2-8  
 PRESET ..... 3-14, 3-42  
 PREV ..... 3-11, 3-35  
 PREVIOUS PAGE ..... 3-8, 3-27  
 Print paper ..... 1-2  
 printer ..... 3-13, 3-39  
 Product Overview ..... 1-1  
 Program Code ..... 4-5  
 PULSE ..... 3-6, 3-20

**[Q]**

QUIET ON/OFF ..... 3-13, 3-41

- [R]**
- Reading Data ..... 2-61
- Rear Panel ..... 2-11
- RECALL ..... 3-12, 3-38
- RECALL Key ..... 3-38
- RECALL MEAS 1 ..... 3-12, 3-38
- RECALL MEAS 2 ..... 3-12, 3-38
- RECALL MEAS 3 ..... 3-12, 3-38
- recall meas data ..... 3-12, 3-38
- RECALL MEM/FDD ..... 3-12, 3-38
- RECALL OFFSET ON/OFF ..... 3-14, 3-43
- RECALL REF DATA ..... 3-12, 3-38
- RECOVER ..... 3-12, 3-37
- REF LEVEL ..... 3-5
- REF LEVEL Key ..... 3-17
- REFERENCE ..... 3-1, 3-8, 3-29
- RELATIVE ..... 3-8, 3-28
- REMOTE CONTROL ..... 4-1
- REPEAT ..... 3-7
- REPEAT Key ..... 3-23
- Replacing and Cleaning the  
Optical-Connector Adapter of Q8384 .... 1-11
- RESOLUTION ..... 3-6
- RESOLUTION Key ..... 3-19
- RIGHT PEAK ..... 3-10, 3-34
- RMS ..... 3-8, 3-25, 5-4
- [S]**
- S.IMPOSE ON/OFF ..... 3-11, 3-35
- Sample Programs for Setting or Reading  
Measurement Conditions ..... 4-41
- SAMPLING POINT ..... 3-10, 3-33
- sampling point ..... 3-11, 3-35
- SAVE ..... 3-12, 3-37
- SAVE Key ..... 3-37
- SAVE MEAS 1 ..... 3-7, 3-12, 3-24, 3-37
- SAVE MEAS 2 ..... 3-12, 3-37
- SAVE MEAS 3 ..... 3-8, 3-12, 3-37
- save meas data ..... 3-12, 3-37
- SAVE MEM 3 ..... 3-27
- SAVE MEM/FDD ..... 3-12, 3-37
- SAVE Pin→REF DATA ..... 3-8, 3-27
- SAVE REF DATA ..... 3-7, 3-12, 3-24, 3-37
- Saving Data ..... 2-60
- Saving or Reading Data ..... 2-59
- SC connector ..... 1-2
- Screen Annotation ..... 2-9
- Secondary Diffracted Light ..... 5-21
- select output ..... 3-13, 3-39
- Selecting Color Patterns on the Screen ... 2-58
- SELF TEST ..... 3-14, 3-42
- Setting Date/Time ..... 2-58
- Setting the print paper ..... 1-9
- SINGLE ..... 3-7
- SINGLE Key ..... 3-23
- smoothing ..... 3-6, 3-22
- SNR ..... 3-8, 3-9, 3-28, 3-30, 5-8
- SNR Lower Lmt. .... 3-9, 3-31
- SPAN ..... 3-5, 3-16
- SPAN Key ..... 3-16
- SPE DIV ..... 5-11
- SPECIFICATIONS ..... 6-1
- spectral width ..... 3-8, 3-25
- ST connector ..... 1-2
- Standard Accessories ..... 1-2
- START ..... 3-5, 3-7, 3-16, 3-23
- State Changes According to the  
Commands ..... 4-27
- Status Byte ..... 4-28
- STOP ..... 3-5, 3-7, 3-16
- STOP Key ..... 3-23
- Storing ..... 1-10
- Stray Light ..... 5-21
- sweep average ..... 3-6, 3-22
- SWEEP MODE ..... 3-6
- SWEEP MODE Key ..... 3-20
- SYNC HI/LOW ..... 3-6, 3-20
- System Checkout ..... 1-8
- [T]**
- Talker Formats ..... 4-6
- TBL CONT TIME/CH ..... 3-9, 3-29
- TECHNICAL NOTES ..... 5-1
- Threshold Level ..... 3-8, 3-9, 3-27, 3-28, 3-31
- THRESHOLD LVL1(dB) ..... 3-8, 3-25
- THRESHOLD LVL2(dB) ..... 3-8, 3-25
- Time Interval ..... 3-9, 3-30
- TRACE MAX ..... 3-11, 3-35
- TRANS ..... 3-7, 3-24
- Transporting ..... 1-12
- [U]**
- UNDO ..... 3-14, 3-44

Alphabetical Index

Using Expanded Functions and  
Inputting/Outputting Data ..... 2-57

**[W]**

Warm-up time ..... 1-12  
WARNING ON/OFF ..... 3-13, 3-41  
WAVE/FREQ nm/THz ..... 3-5, 3-16  
wdm ..... 3-8, 3-28  
WDM ASE Method ..... 3-8, 3-9,  
3-27, 3-28,  
3-31  
WDM Light Signal Characteristic  
Analysis ..... 2-37  
wdm monitor ..... 3-8, 3-29  
WIDTH ..... 3-8, 3-25,  
3-26

**[X]**

X-CHANGE UPR/LOW ..... 3-11, 3-35  
XdB WIDTH ..... 3-8, 3-26,  
5-6  
Xnm LEVEL ..... 3-8, 3-25,  
3-26  
Xnm Level ..... 5-5, 5-7

**[Y]**

YEAR ..... 3-13, 3-40

ADVANTEST product is warranted against defects in material and workmanship for a period of one year from the date of delivery to original buyer.

## LIMITATION OF WARRANTY

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by buyer, unauthorized modification or misuse, accident or abnormal conditions of operations.

No other warranty is expressed or implied. ADVANTEST specifically disclaims the implied warranties of merchantability and fitness for a particular purpose.

ADVANTEST shall not be liable for any special incidental or consequential damages, whether in contract, tort or otherwise.

Any and all warranties are revoked if the product is removed from the country in which it was originally purchased.

## SERVICE

During the warranty period, ADVANTEST will, at its option, either repair or replace products which prove to be defective.

When trouble occurs, buyer should contact his local supplier or ADVANTEST giving full details of the problem and the model name and serial number.

For the products returned to ADVANTEST for warranty service, buyer shall prepay shipping and transportation charges to ADVANTEST and ADVANTEST shall pay shipping and transportation charges to return the product to buyer. However, buyer shall pay all charges, duties, and taxes incurred in his country for products returned from ADVANTEST.

## CLAIM FOR DAMAGE IN SHIPMENT TO ORIGINAL BUYER

The product should be thoroughly inspected immediately upon original delivery to buyer. All material in the container should be checked against the enclosed packing list or the instruction manual alternatively. ADVANTEST will not be responsible for shortage unless notified immediately.

If the product is damaged in any way, a claim should be filed by the buyer with carrier immediately. (To obtain a quotation to repair shipment damage, contact ADVANTEST or the local supplier.) Final claim and negotiations with the carrier must be completed by buyer.

## SALES & SUPPORT OFFICES

Advantest(Singapore)Pte.Ltd.

438A Alexandra Road

#08-03/06 Alexandra Technopark Singapore 119967

Phone : 65-274-3100 Facsimile : 65-274-4055

ROHDE & SCHWARZ Engineering and Sales GmbH

Mühdorfstr. 15 (P.O.B. 80 1429, D-81614 München)

D-81671 München, Germany

Phone : 49-89-4129-13711 Facsimile : 49-89-4129-13723

TEKTRONIX INC.

P.O. Box 500, M/S 39-520, Beaverton, Oregon 97077-0001

or

Howard Vollum Industrial Park, M/S 58-743, Beaverton, OR, 97077, U.S.A.

Inside the U.S. 1-800-426-2200

Outside the U.S. 1-503-627-1933

— Technology Support on the Leading Edge —

# ADVANTEST®

ADVANTEST CORPORATION

Shinjuku-NS Building, 4-1, Nishi-Shinjuku 2-chome, Shinjuku-ku, Tokyo 163-0880, Japan  
Phone:+81-3-3342-7500 Facsimile:+81-3-5322-7270 Telex:232-4914 ADVAN J