



ACL1000/ACL2000

Refrigerant
Leak Detectors

Owner's Manual

BOTH MODELS ARE:

DESIGN CERTIFIED BY

MET LABORATORIES, INC. TO MEET

SAE J1627 FOR R134a, R12 AND R22.

CLASS 1 DIVISION 2 GROUPS
C & D HAZARDOUS
LOCATIONS
HAND HELD
GAS DETECTOR
CLASSIFIED BY
UNDERWRITERS
LABORATORIES,
INC.® AS TO FIRE ELECTRICAL
SHOCK AND EXPLOSION HAZ-
ARDS ONLY. READ OWNERS
MANUAL BEFORE OPERATING.
CAUTION: TO REDUCE THE
RISK OF ELECTRIC SHOCK, DE-
ENERGIZE UNIT BEFORE RE-
PLACING SENSING TIP OR
SERVICING UNIT, USE ONLY
WITH 1.5V ALKALINE BATTER-
IES, SIZE C.



TABLE OF CONTENTS



General Description	2
Features	2
Parts & Controls	3
Getting Started	3
Installing Batteries	3
Operating Features	4
Constant Power Indication	4
Automatic Circuit/Reset	4
Sensitivity Adjustment.....	4
Operating Instructions	5
Operating Tips	5
Applications	7
Maintenance	7
Replacement Parts	8
Specifications	9
Warranty	9

GENERAL INFORMATION



Thank you for purchasing the MAC TOOLS Refrigerant Leak Detector. The advanced micro-processor is at the heart of the ACL1000 and 2000. It permits more advanced management of the circuitry and sensing tip signal than ever before possible. Additionally, the number of components used in the circuit is reduced 50%, increasing reliability and efficiency. The micro-processor monitors the sensing tip and battery voltage levels 4000 times per second, compensating for even the most minor fluctuations in signal. This translates into a stable and dependable tool in almost any environment.

Convenience features have been added to enhance usability. A revolutionary new case design gives the user grip and control, and places the visual indicators (ACL2000) in direct sight during use.

Please take a few moments to read through the following pages, in order to understand and benefit from all the capabilities of your new ACL2000 or ACL1000. We trust that you will be 100% satisfied with your new purchase. If you have any questions or comments after reviewing the manual, please feel free to contact us toll free at (800) 327-5060.

FEATURES



Both Models Feature:

- Microprocessor controlled circuit with Advanced Digital Signal Processing
- Detect ALL Halogenated refrigerants
- Rubber cushion grip
- Certified to SAE J1627 for R12, R22 & R134a
- Variable frequency audible alarm
- Constant Power Indication
- Cordless and portable, operate on 2 C-cell batteries
- 14" (35.5cm) flexible stainless probe
- Spare sensing tip included
- UL Classified for Intrinsic Safety
- CE Approved
- Carrying case included, optional holster and reference leak source
- Two Year Warranty

Additional Features of ACL1000

- Single switch control

Additional Features of ACL2000

- Six segment visual leak size indicator
- True mechanical pump provides positive airflow through sensing tip
- High and Low sensitivity levels
- One touch reset
- Tactile keypad controls
- Real time sensitivity adjustment

PARTS & CONTROLS


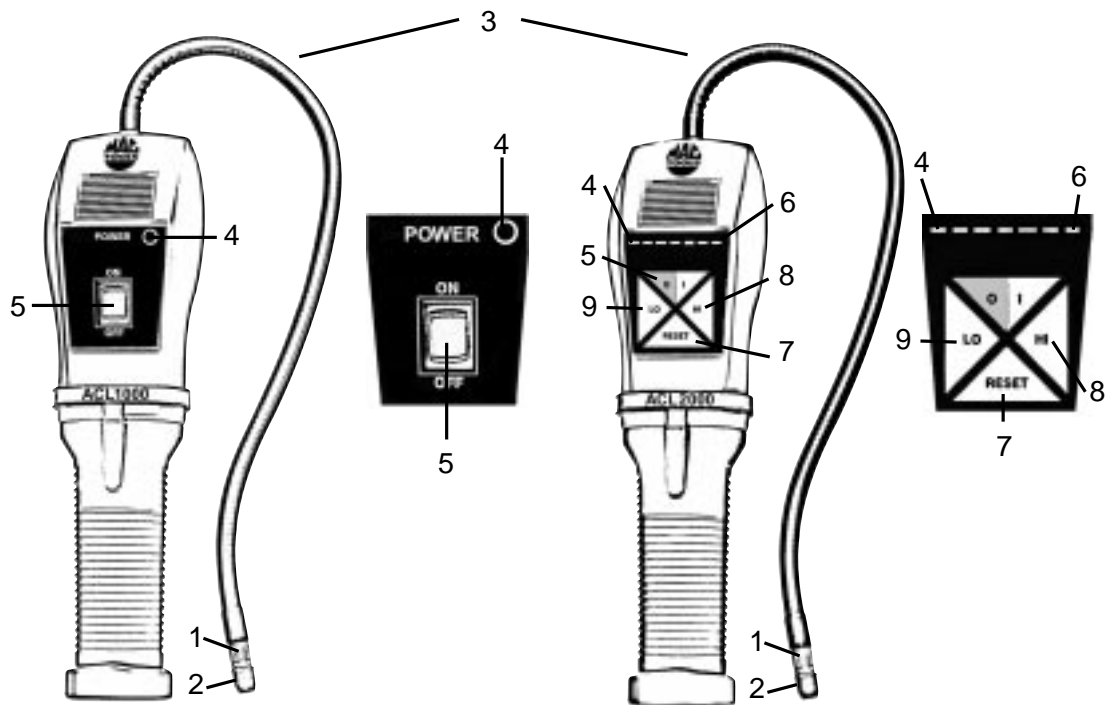


Fig.1

- 1 Sensing Tip
- 2 Tip Protector
- 3 Flexible Probe
- 4 Constant Power Indicator
- 5 Power On/Off
- 6 LED Leak Indicators (ACL2000)
- 7 Reset Button (ACL2000)
- 8 High Sensitivity (ACL2000)
- 9 Low Sensitivity (ACL2000)

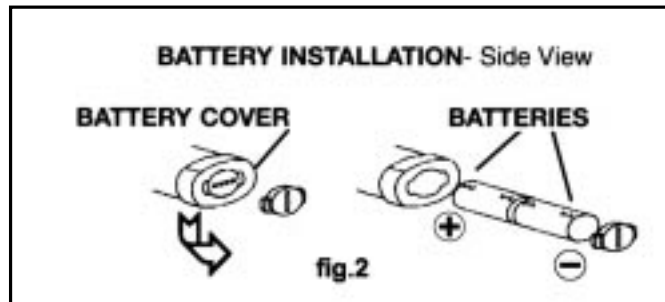

GETTING STARTED

Installing Batteries

1. Remove the battery compartment door located on the bottom of the unit, as shown above. Install batteries, Positive Polarity towards the unit (See Figure 1).

OPERATING FEATURES



Constant Power Indication

The Constant Power indicator allows the user to see the battery level at all times.

ACL1000- The Red LED will remain on whenever the unit is powered on. If the LED is dim, or is not lit, this is an indication that the batteries should be replaced.

ACL2000 - The first LED (leftmost) in the bargraph will remain on whenever the unit is powered on. If the LED is dim, or is not lit, this is an indication that the batteries should be replaced.

Automatic Circuit/Reset Feature

Both detectors feature an Automatic circuit that sets the unit to ignore ambient concentrations of refrigerant. The ACL2000 additionally features a Reset function key for convenience.

- Automatic Circuit - Upon initial power on, the unit automatically sets itself to ignore the level of refrigerant present at the tip. Only a level, or concentration, greater than this will cause an alarm.

CAUTION: Be aware that this feature will cause the unit to ignore any refrigerant present at turn on. In other words, with the unit off if you place the tip up to a known leak and switch the unit on, no leak will be indicated!

- Reset Feature - Resetting the unit during operation performs a similar function, it programs the circuit to ignore the level of refrigerant present at the tip. This allows the user to 'home-in' on the source of the leak (higher concentration). Similarly, the unit can be moved to fresh air and reset for maximum sensitivity. Resetting the unit with no refrigerant present (fresh air) causes any level above zero to be detected.

To Reset the unit:

ACL1000 - Switch the unit OFF and back ON again

ACL2000 - Press the RESET key. Whenever the unit is reset, all LED's will light for 1 second. This provides a visual confirmation of the reset action.

Sensitivity Adjustment (ACL2000 Only)

The ACL2000 provides two levels of sensitivity. The base beeping tone is an indication of sensitivity level; the quicker beep rate indicates a higher level. When the unit is switched on, it is set to the high sensitivity position.

1. To change the sensitivity, press the LO key. When the key is pressed, the visual display will momentarily show the four left LED's red. The base beep rate will slow, indicating Low Sensitivity level.
2. To switch back to High Sensitivity, press the HI key. The three right LED's will light momentarily, and the base beep rate quickens.

OPERATING INSTRUCTIONS



1. Switch the unit on:
ACL1000 - Move the ON/OFF switch to the ON position.
ACL2000 - Press the "I/O" (Red and Green) key. All LED's will light for two seconds as the unit performs a self check.
2. The unit will begin beeping at a steady rate.
3. Verify the battery level by observing the constant power indicator (see above).
4. Begin searching for leaks. When refrigerant is detected, the audible tone will change to a 'siren' type sound, distinctly different from the base beep rate.
ACL2000 - Additionally, the visual indicators will light progressively as described in the Alarm Indications section.
5. **ACL2000** - Sensitivity can be adjusted at any time during operation by using the HI or LO keys.
6. If a full alarm occurs before the leak is pinpointed, RESET the unit as described above, to reset the circuit to a zero reference.

OPERATING TIPS



The following section includes several general operating tips, and the SAE J1628 recommended procedure for leak detection.

1. In areas that are heavily contaminated with gas, the unit may be reset to block out ambient concentrations of gas. The probe should not be moved while the unit is being reset. The unit can be reset as many times as needed.
2. In windy areas, even a large leak can be difficult to find. Under these conditions, it is best to shield the potential leak area.
3. Be aware that the detector may alarm if the sensing tip comes in contact with moisture and/or solvents. Therefore, avoid contact with these when leak checking.

SAE J1628 Recommended Procedure


NOTE: On Automotive A/C Systems, test with the engine not in operation.

1. The air conditioning or refrigeration system should be charged with sufficient refrigerant to have a gauge pressure of at least 340 kPa (50 psi) when not in operation. At temperatures below 15° C (59° F) leaks may not be measurable, since this pressure may not be reached.
2. Take care not to contaminate the detector probe tip if the part being tested is contaminated. If the part is particularly dirty, or condensate (moisture) is present it should be wiped off with a dry shop towel or blown off with shop air. No cleaners or solvents should be used, since the detector may be sensitive to their ingredients.
3. Visually trace the entire refrigerant system, and look for signs of air conditioning lubricant leakage, damage, and corrosion on all lines, hoses, and components. Each questionable area should be carefully checked with the detector probe, as well as all fittings, hose to line couplings, refrigerant controls, service ports with caps in place, brazed or welded areas, and areas around attachment points and hold-downs on lines and components.

OPERATING TIPS



4. Always follow the refrigerant system around in a continuous path so that no areas of potential leaks are missed. If a leak is found, always continue to test the remainder of the system.
5. At each area checked, the probe should be moved around the location, at a rate no more than 25 to 50 mm/second (1-2 in/second), and no more than 5 mm (1/4 in) from the surface, completely around the position. Slower and closer movement of the probe greatly improves the likelihood of finding a leak (see Fig. 2, below). Any increase in beep rate is indicative of a leak.

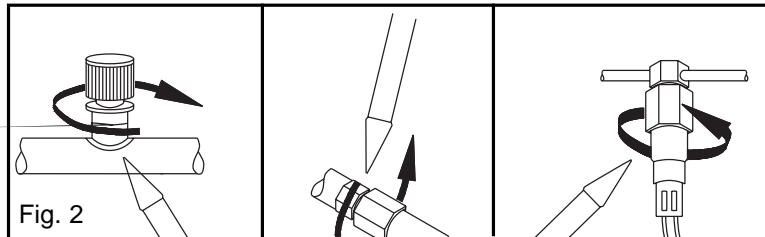

6. An apparent leak shall be verified at least once as follows:
 - a) Blow shop air into the area of the suspected leak, if necessary, and repeat the check of the area. In cases of very large leaks, blowing out the area with shop air often helps locate the exact position of the leak.
 - b) First move the probe to fresh air and reset. Then hold the probe tip as close as possible to the indicated leak source and slowly move around it until the leak is confirmed.

Automotive A/C Systems only -

7. Leak testing of the evaporator core while in the air conditioning module shall be accomplished by turning the air conditioning blower on high for a period of 15 seconds minimum, shutting it off, then waiting for the refrigerant to accumulate in the case for 10 minutes.
After such time, insert the leak detector probe into the blower resistor block or condensate drain hole, if no water is present, or into the closest opening in the heating/ventilation/air conditioning case to the evaporator, such as the heater duct or a vent duct. If the detector alarms, a leak apparently has been found.

All Systems -

8. Following any service to the refrigerant system and any other service which disturbs the refrigerant system, a leak test of the repair and of the service ports of the refrigerant system should be done.

APPLICATIONS



Both of the Leak Detectors covered by this manual may be used to:

- Detect refrigerant gas leaks in Air Conditioning or Refrigeration systems and storage/recover containers. These detectors will respond to ALL halogenated (contains Chlorine or Fluorine) refrigerants. This includes, but is not limited to:
 - CFCs e.g. R12, R11, R500, R503 etc...
 - HCFCs e.g. R22, R123, R124, R502 etc...
 - HFCs e.g. R134a, R404a, R125 etc...
 - Blends such as AZ-50, HP62, MP39, R410a etc...
- Detect Ethylene Oxide gas leaks in hospital sterilizing equipment (detects halogenated propellant)
- Detect SF-6 in high voltage circuit breakers
- Detect most gases that contain Chlorine, Fluorine and Bromine (halogen gases)
- Detect cleaning agents used in dry cleaning applications such as perchloroethylene.
- Detect Halon gases in fire extinguishing systems

MAINTENANCE



Proper maintenance of your Leak Detector is very important. Carefully following the instructions, outlined below, will reduce performance problems and increase the life expectancy of the unit.

WARNING: TURN UNIT OFF BEFORE REPLACING THE SENSING TIP. FAILURE TO DO SO MAY RESULT IN A MILD ELECTRICAL SHOCK!

Keep the sensing tip clean: Prevent dust, moisture and grease build-up by utilizing the provided tip protector. Never use the unit without the protector in place.

Before using the unit always inspect the tip and protector to see that they are free of dirt and/or grease. To clean:

1. Remove protector by grasping and pulling off tip.
2. Clean protector with shop towel and/or compressed air.
3. If the tip itself is dirty it can be cleaned by immersing in a mild solvent, such as alcohol, for a few seconds, and then using compressed air and/or a shop towel to clean.

NOTE: Never use solvents such as gasoline, turpentine, mineral spirits, etc... as these will leave a detectable residue and desensitize your unit.

Sensing tip replacement: The tip will eventually wear out and require replacement. It is difficult to predict exactly when this will occur since tip longevity is directly related to the conditions and frequency of use. The tip should be replaced whenever the alarm sounds or becomes erratic, in a clean, pure, air environment.

MAINTENANCE



To replace the tip:

1. Make sure the unit is OFF.
2. Remove the old tip by unscrewing counter-clockwise.
3. Use the supplied replacement tip, located in the carrying case. Replace by screwing on clockwise.

REPLACEMENT PARTS



Standard Equipment

Your Halogen Leak Detector comes equipped with one Carrying Case, one Owner's Manual, and one replacement Sensing Tip.

To purchase replacement parts for you leak detector please contact your local distributor. To ensure that you obtain the correct parts it is best to reference the part number when placing your order.

Replacement Parts

Part #	Part Description
TIFXP-2RED	Maintenance Kit 3 Sensing Tips 3 Tip Protectors
TIFXP-4AMAC	Blow Molded Carrying Case
TIF5201	Reference Leak Source

SPECIFICATIONS

Power Supply:	3V DC; two "C" cell Alkaline batteries
Maximum Sensitivity:	Per SAE J1627 Rating Criteria Certified @ 0.5 oz/yr. (14gr/yr)
Ultimate sensitivity	
ACL1000	less than 0.4 oz/yr (11 gr/yr) for all Halogen based refrigerants.
ACL2000	less than 0.25 oz/yr (7 gr/yr) for all Halogen based refrigerants.
Sensing Tip Life:	Approximately 20 hours
Operating Temperature:	30° -125° F (0° to 52° C)
Battery Life:	
ACL1000:	Approximately 40 hours normal use
ACL2000:	Approximately 30 hours normal use
Duty Cycle:	Continuous, no limitation
Response Time:	Instantaneous
Reset Time:	One second
Warm-Up Time:	Approximately 2 Seconds
Unit Weight:	1.2 pounds (560 grams) (with batteries)
Unit Dimensions:	9" x 2.5" x 2.5" (22.9cm x 6.5cm x 6.5cm)
Probe Cord Length:	14" or 35.5 cm

WARRANTY & REPAIR

This instrument has been designed and manufactured to provide unlimited service. Should the unit be inoperative, after performing the recommended maintenance, a no-charge repair or replacement will be made to the original purchaser if the claim is made within TWO years from the date of purchase. This warranty applies to all repairable instruments that have not been tampered with or damaged through improper use. This warranty does not cover batteries, sensing tips, tip protectors, or any other materials that wear out during normal operation of the instrument.

Before returning your instrument for repair please make sure that you have carefully reviewed the Unit Maintenance section of this manual to determine if the problem can be easily fixed. Make sure that you have either replaced or cleaned the sensing tip and tip protector and that the batteries are working properly BEFORE returning the unit. If the instrument still fails to work properly please call the Customer service Department for RMA number at the Toll Free number below. Repaired or replaced tools will carry an additional 90 day warranty.
For more information please call (800) 327-5060.



Designed & Engineered in the USA
Manufactured in China

Toll Free Customer Service: 1-800-327-5060