

# Manual Supplement

Manual Title: 116C Users  
Part Number: 2538707  
Print Date: July 2006  
Revision/Date:

Supplement Issue: **5**  
Issue Date: 1/07  
Page Count: 6

---

---


This supplement contains information  
necessary to ensure the accuracy of  
the above manual.

## Change #1

On page 3, add the following after the last bullet:

- **Do not use the Auto Volts function to measure voltages in circuits that could be damaged by this function's low input impedance ( $\approx 3 \text{ k}\Omega$ ).**

On page 13, replace the figure with the following:

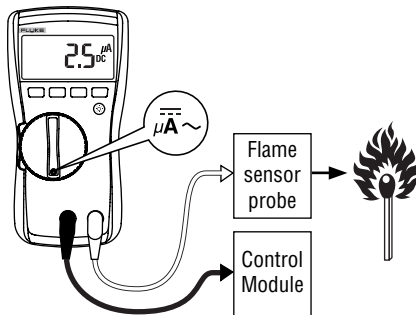

## Change #2

On page 17, under **General Specifications**, replace the first sentence with the following:

Accuracy is specified for 1 year after calibration, at operating temperatures of 18 °C to 28 °C, with relative humidity at 0 % to 90 %.

## Change #3

On page 18, change the following:

From: **IP Rating** (dust and water protection)...IP52 with no vacuum applied

To: **IP Rating** (dust and water protection)...IP42

## Change #4, 38186

On page 2, add the following bullet:

- **Only use test leads that have the same voltage, category, and amperage ratings as the meter and that have been approved by a safety agency.**

On page 20, Table 1, replace footnote 3 with the following:

[3] Frequency is ac coupled and specified from, 5 Hz to 50 kHz.

## Change #5, 39102

On page 19, Table 1, for the Ohms **Function**, change the 40.00 M $\Omega$  Accuracy:

From: 1.5% + 2

To: 5% + 2

## Change #6

On page 15, replace the figure with the following:

