


## Oscilloscope Calibration Options for Fluke 5500A/5520A Multi-Product Calibrators

Extended Specifications  
November 1999

### General Specifications

These specifications apply to the 5520A-SC1100, 5500A-SC600 and 5500A-SC300 Oscilloscope Calibration Options. General specifications for the 5500A and 5520A can be found in the 5500A/5500A Extended Specifications (order publication number 1264848). The specifications are valid when the calibrator is operated under the conditions specified in the operator manual, and has completed a warm-up period of at least twice the length of time the calibrator was powered off, up to a maximum of 30 minutes.

The 5520A-SC1100 can only be installed in a 5520A calibrator. The 5500A-SC600 and SC300 can be installed in a 5520A or a 5500A calibrator.

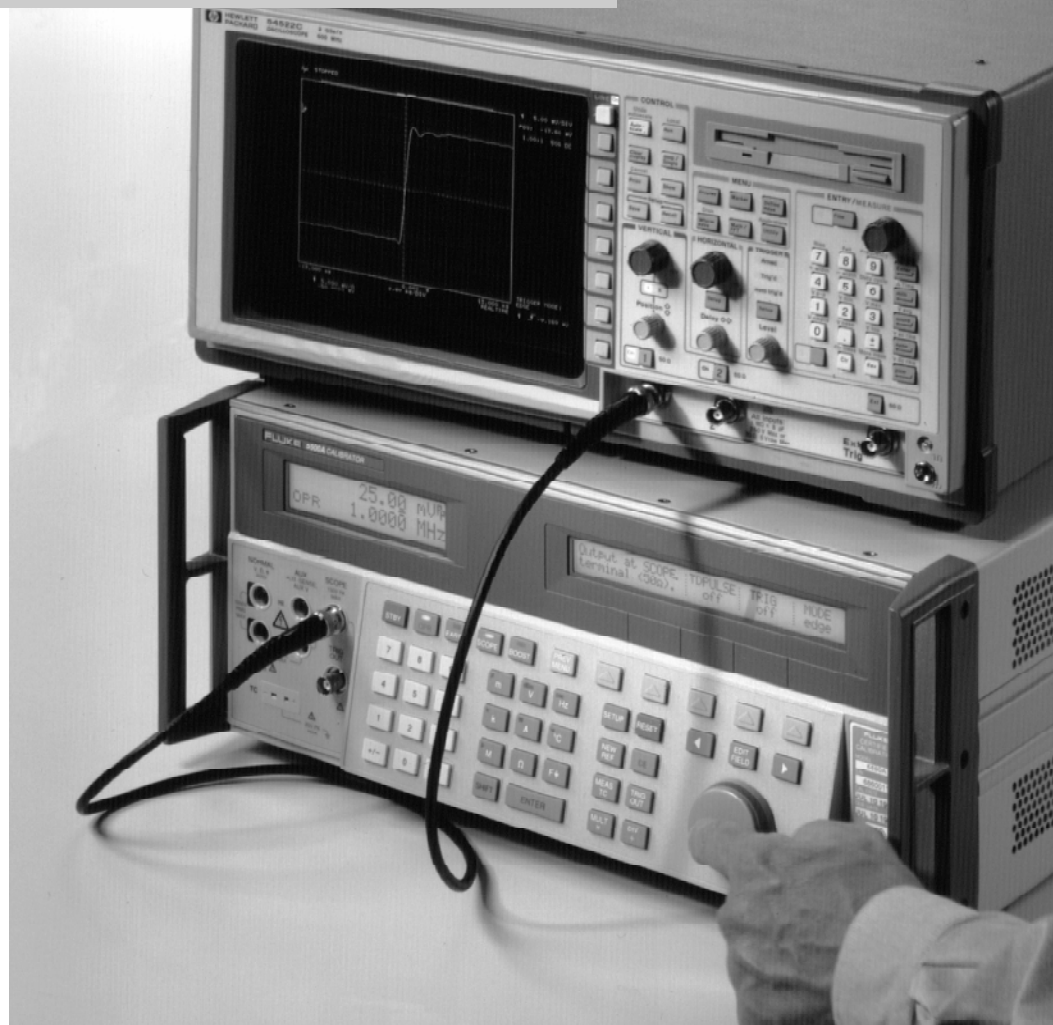

# Voltage Function Specifications

## 5520A-SC1100 and 5500A-SC600

Volt Function		DC Signal		Square Wave Signal <sup>1</sup>	
Load		Into 50Ω	Into 1 MΩ	Into 50Ω	Into 1 MΩ
<b>Amplitude Characteristics</b>					
Range		0V to ±6.6V	0V to ±130V	±1 mV to ±6.6V p-p	±1 mV to ±130V p-p
	Range	Resolution			
Resolution	1 mV to 24.999 mV 25 mV to 109.99 mV 110 mV to 2.1999V 2.2V to 10.999V 11V to 130V	1 μV 10 μV 100 μV 1 mV 10 mV			
Adjustment Range		Continuous			
1-Year Absolute Uncertainty, tcal ± 5°C		± (0.25% of output + 40 μV)	± (0.05% of output + 40 μV)	± (0.25% of output + 40 μV)	± (0.1% of output + 40 μV) <sup>2</sup>
Sequence		1-2-5 (e.g., 10 mV, 20 mV, 50 mV)			
<b>Square Wave Frequency Characteristics</b>					
Range		10Hz to 10 kHz			
1-Year Absolute Uncertainty, tcal ± 5°C		± (2.5 ppm of setting)			
Typical Abberation (from 50% of leading/trailing edge) 25 mV to 130V: within 4 μs 10 mV to 25 mV: within 8 μs 1 mV to 10 mV: within 14 μs		< (0.5% of output + 100 μV)			

<sup>1</sup> Positive or negative, zero referenced square wave.

<sup>2</sup> Above 1 kHz, ± (0.25% of output + 40 μV). Assumes connectors and cables are in good condition.

## 5500A-SC300

Volt Function		DC Signal		Square Wave Signal <sup>1</sup>	
Load		Into 50Ω	Into 1 MΩ	Into 50Ω	Into 1 MΩ
Amplitude Range		0V to ±2.2V	0V to ±33V	±1.8 mV to ±2.2V p-p	±1.8 mV to ±105V p-p
1-Year Absolute Uncertainty, tcal ± 5°C		± (0.25% of output + 100 μV)			
Sequence		1-2-5 (e.g., 10 mV, 20 mV, 50 mV)			
Frequency Range		10 Hz to 10 kHz			

<sup>1</sup> Positive or negative, zero referenced square wave.

# Edge Function Specifications

## 5520A-SC1100 and 5500A-SC600

Edge Characteristics into 50Ω		1-Year Absolute Uncertainty, tcal ±5°C
<b>Amplitude</b>		
Rise Time	< 300 ps	+ 0/-100 ps
Range (p-p)	5.0 mV to 2.5V	± (2% of output + 200 μV)
Resolution	4 digits	
Adjustment Range	± 10% around each sequence value (indicated below)	
Sequence Values	5 mV, 10 mV, 25 mV, 50 mV, 60 mV, 80 mV, 100 mV, 200 mV, 250 mV, 300 mV, 500 mV, 600 mV, 1V, 2.5V	
<b>Other Edge Characteristics</b>		
Frequency Range	1 kHz to 10 MHz <sup>1</sup>	± (2.5 ppm of setting)
Frequency Range	≤ 300 ps <sup>1</sup>	(+ 0 ps/-100ps)
Typical Jitter, Edge to Trigger	< 5 ps [p-p]	
Leading Edge Aberrations <sup>2</sup>	within 2 ns from 50% of rising edge]	< (3% of output + 2 mV)
	2 ns to 5 ns	< (2% of output + 2 mV)
	5 ns to 15 ns	< (1% of output + 2 mV)
	after 15 ns	< (0.5% of output + 2 mV)
Typical Duty Cycle	45% to 55%	
Tunnel Diode Pulse Drive	Square wave at 100 Hz to 100 kHz, with variable amplitude of 60V to 100V p-p	
Tunnel Diode Option	≤ 125 ps @ 250 mV p-p	

<sup>1</sup> Frequency range above 2 MHz has rise time specification ≤350 ps.

<sup>2</sup> Below 250 mV aberrations are typical.

## 5500A-SC300

Edge Characteristics into 50Ω		1-Year Absolute Uncertainty, tcal ±5°C
Amplitude Range (p-p)	4.5 mV to 2.75V	± (2% of output + 200 μV)
Frequency Range	1 kHz to 1 MHz	± (25 ppm of setting + 15 mHz)
Rise Time	≤1 ns	
Typical Jitter, Edge to Trigger	<5 ps (p-p)	
Leading Edge Aberrations	Within 10 ns	< (2% of output + 2 mV)
	10 to 30 ns	< (1% of output + 2 mV)
	After 30 ns	< (0.5% of output + 2 mV)
Typical Duty Cycle	45% to 55%	

# Leveled Sinewave Function Specifications

## 5520A-SC1100 (> 600 MHz)

Characteristics into 50Ω	Frequency Range	
	50 kHz (reference)	600 MHz to 1.1 GHz
<b>Amplitude Characteristics</b>		
Range	5 mV to 3.5V	
Resolution	< 100 mV: 3 digits; ≥ 100 mV: 4 digits	
<b>Adjustment Range</b>	<b>Continuously Adjustable</b>	
1-Year Absolute Uncertainty, tcal ± 5°C	± (2% of output + 300 μV)	± (7% of output + 300 μV)
Flatness (relative to 50 MHz) <sup>1</sup>	not applicable	± (5% of output + 100 μV)
Short-Term Amplitude Stability	≤ 1 % <sup>2</sup>	
<b>Frequency Characteristics</b>		
Resolution	100 kHz	
1-Year Absolute Uncertainty, tcal ± 5°C	± 2.5 ppm	
<b>Distortion Characteristics</b>		
2 <sup>nd</sup> Harmonic	≤ -33 dBc	
3 <sup>rd</sup> and Higher Harmonic	≤ -38 dBc	

<sup>1</sup> As measured near oscilloscope bandwidth frequency.

<sup>2</sup> Within one hour after reference amplitude setting, provided temperature varies no more than ± 5°C.

## 5520A-SC1100 and 5500A-SC600

Leveled Sine Wave Characteristics into 50Ω	Frequency Range			
	50 kHz (Reference)	50 kHz to 100 MHz	100 MHz to 300 MHz	300 MHz to 600 MHz
<b>Amplitude</b>				
Range (p-p)	5 mV to 5.5V			
1-Year Absolute Uncertainty, tcal ± 5°C	± (2% of output + 300 μV)	± (3.5% of output + 300 μV)	± (4% of output + 300 μV)	± (6% of output + 300 μV)
Flatness (relative to 50 kHz) <sup>1</sup>	Not applicable	± (1.5% of output + 100 μV)	± (2% of output + 100 μV)	± (4% of output + 100 μV)
Short-Term Amplitude Stability	≤ 1% <sup>2</sup>			
<b>Frequency</b>				
Resolution	10 kHz			
1-Year Absolute Uncertainty, tcal ± 5°C	± 2.5 ppm			
<b>Distortion</b>				
2 <sup>nd</sup> Harmonic	≤ -33 dBc			
3 <sup>rd</sup> and Higher Harmonics	≤ -38 dBc			

<sup>1</sup> As measured near oscilloscope bandwidth frequency.

<sup>2</sup> Within one hour after reference amplitude setting, provided temperature varies no more than ± 5°C.

### 5500A-SC300

Leveled Sine Wave Characteristics into 50Ω	Frequency Range		
	50 kHz (Reference)	50 kHz to 100 MHz	100 MHz to 300 MHz <sup>1</sup>
<b>Amplitude</b>			
Range (p-p)		5 mV to 5.5V <sup>1</sup>	
1-Year Absolute Uncertainty, tcal ±5°C	± (2% of output + 200 μV)	± (3.5% of output + 300 μV)	± (4% of output + 300 μV)
Flatness (relative to 50 kHz) <sup>1</sup>	Not applicable	± (1.5% of output + 100 μV)	± (2% of output + 100 μV)
Short-Term Amplitude Stability	≤1% <sup>2</sup>		
<b>Frequency</b>			
Resolution	10 kHz		
1-Year Absolute Uncertainty, tcal ±5°C	± 2.5 ppm		
<b>Distortion</b>			
2nd Harmonic	≤ -33 dBc		
3rd and Higher Harmonics	≤ -38 dBc		

<sup>1</sup> Extended frequency range to 350 MHz is provided, but flatness is not specified. Amplitude is limited to 3V for frequencies above 250 MHz.

<sup>2</sup> Within one hour after reference amplitude setting, provided temperature varies no more than ±5°C.

## Time Marker Function Specifications

### 5520A-SC1100 and 5500A-SC600

Time Marker into 50Ω <sup>1</sup>	5s to 50 ms	20 ms to 100 ns	50 ns to 20 ns	10 ns	5 ns to 2 ns
1-Year Absolute Uncertainty, tcal ±5°C <sup>2</sup>	± (25 + t* X 1000) ppm	± 2.5 ppm	± 2.5 ppm	± 2.5 ppm	± 2.5 ppm
Wave Shape	Spike or square	Spike, square, 20%-pulse	Spike or square	Square or sine	Sine
Typical Jitter (p-p)	<10 ppm	<1 ppm	<1 ppm	<1 ppm	<1 ppm
Sequence	5-2-1 from 5s to 2 ns (e.g., 500 ms, 200 ms, 100 ms)				

<sup>1</sup> Output amplitude >1V pk.

<sup>2</sup> Time marker uncertainty is ± 50 ppm when measured off of cardinal points.

\* t = time in seconds.

### 5500A-SC300

Time Marker into 50Ω [1]	5s to 100 μs	50 μs to 2 μs	1 μs to 20 ns	10 ns to 2 ns
1-Year Absolute Uncertainty, tcal ±5°C	± (25 + t* X 1000) pmm	± (25 + t* X 15000) pmm	± 25 ppm	± 25 ppm
Wave Shape	Pulsed Sawtooth	Pulsed Sawtooth	Pulsed Sawtooth	Sine
Sequence	5-2-1 from 5s to 2 ns (e.g., 500 ms, 200 ms, 100 ms)			

<sup>1</sup> Typical Amplitude > 1V

\* t = time in seconds.

### Trigger Functions 5520A-SC1100, 5500A-SC600 and 5500A-SC300

Available for edge and time marker functions (volt, pulse and video are available for 5520A-SC1100 and 5500A-SC600 only).

# Wave Generator Function Specifications

## 5520A-SC1100, 5500A-SC600 and 5500A-SC300

Wave Generator Characteristics	Square Wave, Sine Wave, and Triangle Wave into 50Ω or 1 MΩ
<b>Amplitude</b>	
Range	Into 1 MΩ: 1.8 mV to 55V p-p Into 50Ω: 1.8 mV to 2.5V p-p (5520A-SC1100 and 5500A-SC600) Into 50Ω: 1.8 mV to 2.2V p-p (5500A-SC300)
1-Year Absolute Uncertainty, tcal ±5°C 10 Hz to 10 kHz	± (3% of p-p output + 100 μV)
Sequence	1-2-5 (eg., 10 mV, 20 mV, 50 mV,...)
Typical DC Offset Range	0 to ± (≥40% of p-p amplitude) <sup>1</sup>
<b>Frequency</b>	
Range	10 Hz to 100 kHz
Resolution	4 or 5 digits depending on frequency

<sup>1</sup> The DC offset plus the wave signal must not exceed 30V rms.

# Pulse Generator Function Specifications

## 5520A-SC1100 and 5500A-SC600

The pulse generator is designed for oscilloscope capture function tests and trigger verification applications.

Pulse Generator Characteristics	Positive Pulse into 50Ω
Typical Rise/Fall Times	2 ns
Amplitude Available	Discrete steps: 2.5V, 1V, 250 mV, 100 mV, 25 mV, 10 mV
<b>Pulse Width<sup>1</sup></b>	
Range	4 ns to 500 ns <sup>1</sup>
Uncertainty <sup>2</sup>	5% ± 2 ns
<b>Pulse Period</b>	
Range	20 ms to 200 ns (50 Hz to 6.6 MHz)
1-Year Absolute Uncertainty, tcal ± 5°C	± 2.5 ppm

<sup>1</sup> Pulse width not to exceed 40% of period.

<sup>2</sup> Pulse width uncertainty for periods less than 2 μs are not specified.

# TV Trigger Specifications

**5520A-SC1100 and 5500A-SC600.** TV Trigger is provided at the Scope Output Terminal

Trigger Signal Type	Parameters
Frame Formats	Selectable NTSC, SECAM, PAL, PAL-M
Polarity	Selectable Inverted or Uninverted Video
Amplitude into 50Ω (p-p)	Adjustable 0 to 1.5V p-p into 50Ω load, (±7% accuracy)
Line Marker	Selectable Line Video Marker

# Input Impedance Measurement Specifications

**5520A-SC1100 and 5500A-SC600**

	Range	Uncertainty
Resistance	40Ω to 60Ω	0.1%
	500 kΩ to 1.5 MΩ	0.1%
Capacitance	5 pF - 50 pF	± (5% of input + 0.5 pF) <sup>1</sup>

<sup>1</sup> Measurements made within 30 minutes of capacitance zero reference. Scope option must be selected for at least five minutes prior to capacitance measurement or zero.

# Overload Measurement Specifications

**5520A-SC1100 and 5500A-SC600.** The overload test function applies dc or ac (1 kHz square wave) power into the 50Ω oscilloscope input and monitors the current. A time measurement counter indicates the time duration of the applied overload signal. When the oscilloscope's input protection circuit reacts and opens up the 50Ω load, the calibrator indication is set to "off" on the right hand display. In order to prevent oscilloscope front end damage, a limited amount of energy is applied by a user settable time limit.

Source Voltage	Time Limit dc or 1 kHz ac
5V to 9V	Settable from 1 Sec to 60 Sec
Typical "On" Current Indication	Typical "Off" Current Indication
5V to 9V	Settable from 1 Sec to 60 Sec

### External Frequency Reference Input (5520A only)

The External Reference Input selection allows the user to provide their own high stability 10 MHz reference clock for the 5500A-SC300, 5500A-SC600 and 5520A-SC1100 when fitted in a 5520A mainframe. All functions except Wave Generator and Marker greater than 50ms are then referenced to the external 10 MHz signal. The external reference input must be between 1V to 5V p-p.

Uncertainty of output = uncertainty of reference + 5 μHz.

# Ordering Information

## Ordering Information

- 5500A** Multi-Product Calibrator
- 5500A/3** Multi-Product Calibrator with 300 MHz Oscilloscope Calibration Option
- 5500A/6** Multi-Product Calibrator with 600 MHz Oscilloscope Calibration Option
- 5520A** High-Performance Multi-Product Calibrator
- 5520A/3** High Performance Multi-Product Calibrator with 300 MHz Oscilloscope Calibration Option
- 5520A/6** High Performance Multi-Product Calibrator with 600 MHz Oscilloscope Calibration Option
- 5520A/1 GHz** High Performance Multi-Product Calibrator with 1.1 GHz Oscilloscope Calibration Option

## Options\*

- 5500A-SC300** 300 MHz/1 ns Oscilloscope Calibration Option
- 5500A-SC600** 600 MHz/300 ps Oscilloscope Calibration Option
- 5520A-SC1100** 1.1 GHz ps Oscilloscope Calibration Option (5520A only)

\* SC options must be installed and calibrated at a Fluke Service Center and include report of calibration.


## Accessories

- 5500A/COIL** 50-Turn Current Coil
- 5500A/CASE** Roll-Aboard Transit Case
- 5500A/LEADS** Comprehensive Test Lead Kit
- 5800A/TDP** 125 ps Tunnel Diode Pulser
- 5520A/HPROBE** Humidity Measurement Probe
- 5500A/HNDL** Side Carry Handle
- Y5537** Rack Mount Kit
- TC100** Test Cart
- 5725A** Amplifier (5500A Only)
- MET/CAL\*** Calibration Software (IEEE and RS232)
- 5500/CAL** Calibration Software (RS232)
- 5800A-7004k** Oscilloscope Cal Cable and Accessory Kit


## Pressure Modules (5520A only)

- FLUKE-700PCK** Pressure Module Calibration Kit (required)
- FLUKE-700P01** Pressure Module 0-10 IN. H<sub>2</sub>O DIFF
- FLUKE-700P02** Pressure Module 0-1 PSID
- FLUKE-700P03** Pressure Module 0-5 PSID
- FLUKE-700P04** Pressure Module 0-15 PSID
- FLUKE-700P05** Pressure Module 0-30 PSIG
- FLUKE-700P06** Pressure Module 0-100 PSIG
- FLUKE-700P07** Pressure Module 0-500 PSIG
- FLUKE-700P08** Pressure Module 0-1000 PSIG
- FLUKE-700P09** Pressure Module 1500 PSIG
- FLUKE-700P22** Pressure Module 0-1 PSID WET
- FLUKE-700P23** Pressure Module 0-5 PSID WET
- FLUKE-700P24** Pressure Module 0-15 PSID WET
- FLUKE-700P29** Pressure Module 3000 PSIG WET
- FLUKE-700P30** Pressure Module 5000 PSIG WET
- FLUKE-700P31** Pressure Module 10000 PSIG WET
- FLUKE-700PA3** Pressure Module 0-5 PSIA
- FLUKE-700PA4** Pressure Module 0-15 PSIA
- FLUKE-700PA5** Pressure Module 0-30 PSIA
- FLUKE-700PA6** Pressure Module 0-100 PSIA
- FLUKE-700PD2** Pressure Module ± 1 PSID
- FLUKE-700PD3** Pressure Module ± 5 PSID

- FLUKE-700PD4** Pressure Module ± 15 PSID
- FLUKE-700PD5** Pressure Module -15+30 PSIG
- FLUKE-700PD6** Pressure Module -15+100 PSIG
- FLUKE-700PD7** Pressure Module -15+200 PSIG
- FLUKE-700PV3** Pressure Module -5 PSID
- FLUKE-700PV4** Pressure Module -15 PSID
- FLUKE-700PMP** Pressure Pump

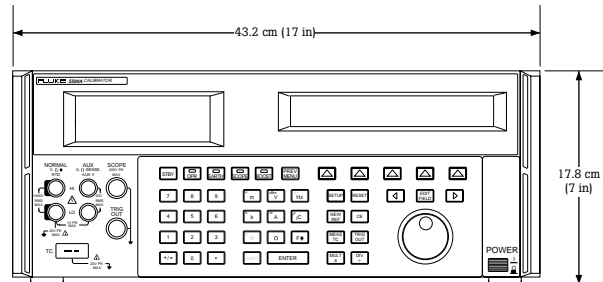

Front view and dimensions.

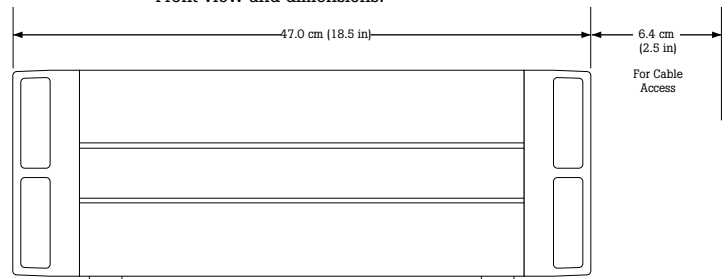

Side view and dimensions.

Note: 5500A and 5520A dimensions are the same.

## Product Compatibility Chart

Model	5520A-SC1100	5500A-SC600	5500A-SC300
5520A	•	•	•
5500A		•	•
5800A/TDP	•	•	

**Fluke.** Keeping your world up and running.

### Fluke Corporation

PO Box 9090, Everett, WA USA 98206

Fluke Europe B.V.  
PO Box 1186, 5602 BD  
Eindhoven, The Netherlands

For more information call:  
U.S.A. (800) 443-5853 or  
Fax (425) 356-5116  
Europe/M-East/Africa (31 40) 2 678 200 or  
Fax (31 40) 2 678 222  
Canada (800) 36-FLUKE or  
Fax (905) 890-6866  
Other countries (425) 356-5500 or  
Fax (425) 356-5116  
Web access: <http://www.fluke.com>



© 1999 Fluke Corporation. All rights reserved.  
Specifications and other product information  
subject to change without notice.  
Printed in U.S.A. 11/99 1265775 D-ENG-N Rev C