

Manual Supplement

Manual Title:	77 Series III Service	Supplement Issue:	3
Part Number:	800604	Issue Date:	8/04
Print Date:	November 1998	Page Count:	2
Revision/Date:	1, 11/99		

This supplement contains information necessary to ensure the accuracy of the above manual.

Change #1

On page 2-4, under Current Conditioning, replace the last sentence with the following:

F1 protects the mA circuitry; F2 protects the 10A circuitry.

Change #2


On page 4-5, Table 4-1, change MP14,

From: 659786

To: 659128

Change #3

On page 2-7, Figure 2-2, replace the bottom half of the figure with the following:

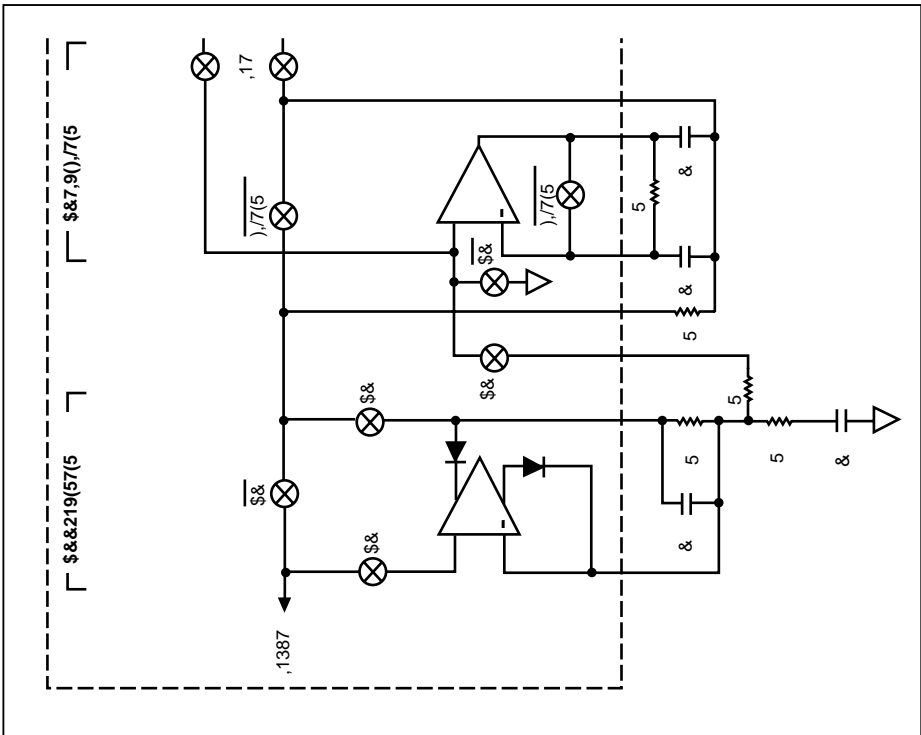

Change #4

On page SAFETY-1, replace the first bullet and add the following:

Change: Never use the meter if the meter or test leads look damaged.

To: Do not use the meter if it is damaged. Before you use the meter, inspect the case. Look for cracks or missing plastic. Pay particular attention to the insulation surrounding the connectors.

Inspect the test leads for damaged insulation or exposed metal. Check the test leads for continuity. Replace damaged test leads before you use the meter.

- If this product is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.
- Before use, verify the meter's operation by measuring a known voltage.
- Avoid working alone.
- Adhere to local and national safety codes. Individual protective equipment must be used to prevent shock and arc blast injury where hazardous live conductors are exposed.

Caution

To avoid possible damage to the meter or to the equipment under test, follow these guidelines:

- **Disconnect circuit power and discharge all high-voltage capacitors before testing resistance, continuity, or diodes.**
- **Use the proper terminals, function, and range for your measurements. Before measuring current, check the meter's fuses and turn power OFF to the circuit before connecting the meter to the circuit.**