

Manual Supplement

Manual Title: Ti20 Users
Print Date: January 2006
Revision/Date:


Supplement Issue: **3**
Issue Date: 9/06
Page Count: 1

This supplement contains information necessary to ensure the accuracy of the above manual. This manual is distributed as an electronic manual on the following CD-ROM:

CD Title:	Ti20 Thermal Imager
CD Rev. & Date:	1, 2/2006
CD PN:	2492146

Change #1

On page 1-11, change **Figure 1-7** as shown below:

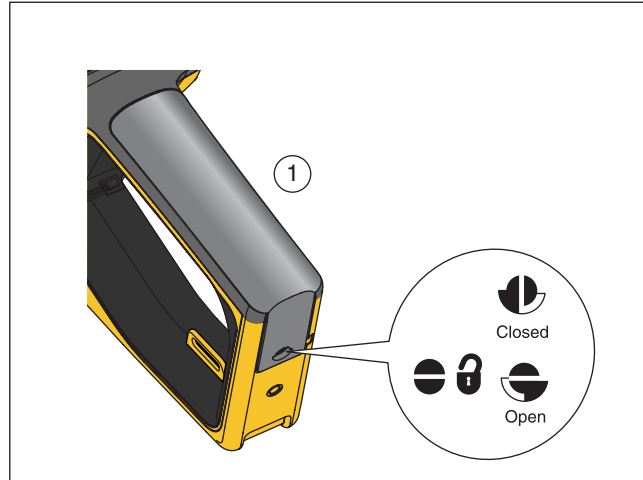

Note that this change also applies to the Quick Reference Guide.

Change #2

On page 2-9, under **Adjusting the Span**, replace the first sentence with the following:

The full temperature range of the Imager is -10 °C to 350 °C (14 °F to 662 °F).

Under step 4, replace the last sentence with the following:

The minimum temperature span is 10 °C.

On page D-1, change the entries for Detector Type, Instantaneous Field of View, Reflected Background Temperature and Relative Humidity to:

Detector Type.....128 x 96 thermal element focal plane array (FPA)

Instantaneous Field of View.....2.7 mrad

Reflected Background Temperature.....-50 to 460 °C (-58 to 860 °F)

Relative Humidity.....10 to 95% noncondensing

On page D-2, under Vibration change the following:

From: MIL-PRF-28800, paragraph 4.5.5.3.1, Class 2

To: MIL-PRF-28800, Class 2