

Synthesized Function Generator

SFG-2000/SFG-2100 Series

USER MANUAL

GW INSTEK PART NO. 82FG-21200MD



ISO-9001 CERTIFIED MANUFACTURER

GW INSTEK

This manual contains proprietary information, which is protected by copyrights. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will company.

The information in this manual was correct at the time of printing. However, Good Will continues to improve products and reserves the rights to change specification, equipment, and maintenance procedures at any time without notice.

Good Will Instrument Co., Ltd.

No. 7-1, Jhongsing Rd., Tucheng City, Taipei County 236, Taiwan.

Table of Contents

SAFETY INSTRUCTIONS	5
Safety Symbols.....	5
Safety Guidelines	6
GETTING STARTED	9
Technical background	10
Lineup/Features.....	12
Front Panel	13
Rear Panel.....	19
Set Up.....	20
Operation Shortcuts	22
Default Setting Contents.....	24
SINE/SQUARE/TRIANGLE WAVE	25
Select the waveform.....	26
Set the Frequency	26
Set the Duty Cycle (Square Waveform)	28
Set Amplitude	29
Set Offset.....	30
TTL CMOS OUTPUT.....	31
Select the waveform.....	32
Set the Frequency	32
Set the Duty Cycle.....	33
Set Amplitude	34
SWEEP.....	35
AMPLITUDE MODULATION	37

FREQUENCY MODULATION	38
COUNTER INPUT	40
STORE/RECALL SETTING	42
APPLICATION EXAMPLES	44
Reference Signal for PLL System	44
Trouble-Shooting Signal Source	44
Transistor DC Bias Characteristics Test.....	45
Amplifier Over-Load Characteristic Test	46
Amplifier Transient Characteristics Test	46
Logic Circuit Test.....	48
Impedance Matching Network Test	48
Speaker Driver Test	49
Sweep for Speaker Test.....	50
FAQ	51
APPENDIX	52
Error Messages	52
Specification.....	53
Declaration of Conformity	55
INDEX	56

SAFETY INSTRUCTIONS

This chapter contains important safety instructions that you must follow when operating SFG-2000 series and when keeping it in storage. Read the following before any operation to insure your safety and to keep the best condition for SFG-2000 series.



Safety Symbols

These safety symbols may appear in this manual or on SFG-2000 series.



WARNING

Warning: Identifies conditions or practices that could result in injury or loss of life.



CAUTION

Caution: Identifies conditions or practices that could result in damage to SFG-2000 series or to other properties.



Attention Refer to the Manual



Earth (ground) Terminal

Safety Guidelines

General Guideline



CAUTION

- Do not place any heavy object on SFG-2000 series.
- Avoid severe impacts or rough handling that leads to damaging SFG-2000 series.
- Do not discharge static electricity to SFG-2000 series.
- Use only mating connectors, not bare wires, for the terminals.
- Do not block or obstruct cooling vent opening.
- Do not perform measurements at power source and building installation site (Note below).
- Do not disassemble SFG-2000 series unless you are qualified as service personnel.

(Note) EN 61010-1:2001 specifies the measurement categories and their requirements as follows. SFG-2000 series falls under category II.

- Measurement category IV is for measurement performed at the source of low-voltage installation.
- Measurement category III is for measurement performed in the building installation.
- Measurement category II is for measurement performed on the circuits directly connected to the low voltage installation.

Power Supply



WARNING

- Input voltage: 115/230V AC +10%, -15%, 50/60Hz
- The power supply voltage should not fluctuate more than 10%.
- Connect the protective grounding conductor of the power cord to earth ground, to avoid electrical shock.

Fuse



WARNING

- Fuse type: T0.125A/ 250V
- Only service personnel are allowed to access internal fuse holders.
- Replace the fuse with the specified type and rating only, for continued fire protection.
- Disconnect the power cord before fuse replacement.
- Make sure the cause of the fuse blowout is fixed before fuse replacement.

Cleaning SFG-2000 series	<ul style="list-style-type: none">• Disconnect the power cord before cleaning.• Use a soft cloth dampened in a solution of mild detergent and water. Do not spray any liquid into SFG-2000 series.• Do not use chemicals or cleaners containing harsh materials such as benzene, toluene, xylene, and acetone.
Operation Environment	<ul style="list-style-type: none">• Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (Note below)• Relative Humidity: < 80%• Altitude: < 2000m• Temperature: 0°C to 40°C
Storage Environment	<p>(Note) EN 61010-1:2001 specifies the pollution degrees and their requirements as follows. SFG-2000 series falls under degree 2. Pollution refers to “addition of foreign matter, solid, liquid, or gaseous (ionized gases), that may produce a reduction of dielectric strength or surface resistivity”.</p> <ul style="list-style-type: none">• Pollution degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence.• Pollution degree 2: Normally only non-conductive pollution occurs. Occasionally, however, a temporary conductivity caused by condensation must be expected.• Pollution degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. In such conditions, equipment is normally protected against exposure to direct sunlight, precipitation, and full wind pressure, but neither temperature nor humidity is controlled. <ul style="list-style-type: none">• Location: Indoor• Relative Humidity: < 80%• Temperature: -10°C to 70°C

Power cord for the United Kingdom

When using SFG-2000 series in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead / appliance must only be wired by competent persons



WARNING: THIS APPLIANCE MUST BE EARTCHED

IMPORTANT: The wires in this lead are coloured in accordance with the following code:

Green/ Yellow: Earth



Blue: Neutral

Brown: Live (Phase)

As the colours of the wires in main leads may not correspond with the colours marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with the letter E or by the earth symbol \oplus or coloured Green or Green & Yellow. The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red.

If in doubt, consult the instructions provided with the equipment or contact the supplier. This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, cable of 0.75mm² should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any moulded mains connector that requires removal /replacement must be destroyed by removal of any fuse & fuse carrier and disposed of immediately, as a plug with bared wires is hazardous if engaged in live socket. Any re-wiring must be carried out in accordance with the information detailed on this label.

GETTING STARTED

This chapter describes SFG-2000 series in a nutshell, including main features and front/rear/display introduction. Follow the Set Up section to properly install and power up SFG-2000 series.



SFG-2000 series overview	Technical background	10
	Series lineup	12
	Main features.....	12
<hr/>		
Panel introduction	Front Panel	13
	Rear Panel.....	19
<hr/>		
Setup	Tilt stand	20
	Power up.....	21
	Recall the default setting	21
	Functionality check	21
<hr/>		
Quick reference	Operation Shortcuts	22
	Default Setting Contents.....	24

Technical background

Traditional function generators

SFG-2000 series uses the latest Direct Digital Synthesis (DDS) technology to generate stable, high resolution output frequency. The DDS technology solves several problems encountered in traditional function generators, as follows.

Constant current circuit methodology


This analog function generating method uses a constant current source circuit built with discrete components such as capacitors and resistors. Temperature change inside the generator greatly affects the components characteristics which lead to output frequency change. The results are poor accuracy and stability.

DDS methodology

In DDS, the waveform data is contained in and generated from a memory. A clock controls the counter which points to the data address. The memory output is converted into analog signal by a digital to analog converter (DAC) followed by a low pass filter. The resolution is expressed as $fs/2k$ where fs is the frequency and k is the control word, which contains more than 28bits. Because the frequency generation is referred to clock signal, this achieves much higher frequency stability and resolution than the traditional function generators.

Block diagram

DDS synthesizer consists of Phase accumulator (counter), lookut table data (ROM), Digital-to-analog converter (DAC), and Low-pass filter (LPF).

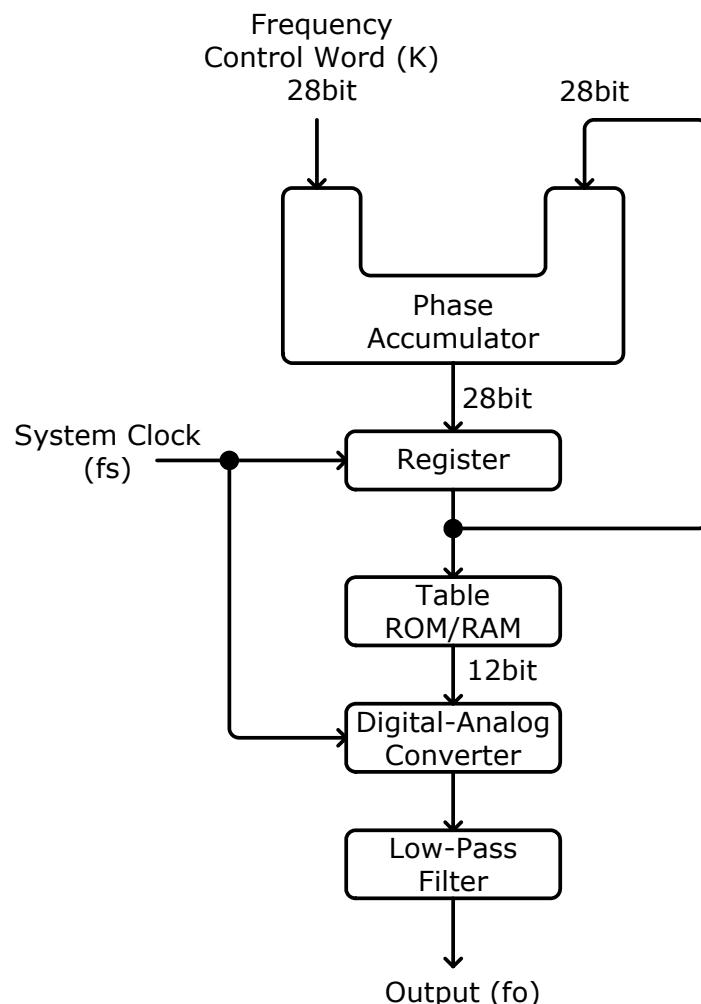

The phase accumulator adds the frequency control word K at every clock cycle f_s . The accumulator output points to a location in the Table ROM/RAM. The DAC converts the digital data into an analog waveform. The LPF filters out the clock frequency to provide a pure waveform.

Lineup/Features

Series lineup


Lineup	Features	Duty cycle	Offset	TTL/ CMOS	Sweep	AM/ FM	Counter
SFG-2004 (4MHz)	●	●	●	—	—	—	—
SFG-2007 (7MHz)	●	●	●	—	—	—	—
SFG-2101 (10MHz)	●	●	●	—	—	—	—
SFG-2102 (20MHz)	●	●	●	—	—	—	—
SFG-2104 (4MHz)	●	●	●	●	●	●	●
SFG-2107 (7MHz)	●	●	●	●	●	●	●
SFG-2110 (10MHz)	●	●	●	●	●	●	●
SFG-2120 (20MHz)	●	●	●	●	●	●	●

Main features


Performance	<ul style="list-style-type: none"> High resolution using DDS and FPGA technology High frequency accuracy: 20ppm Low distortion: -55dBc High resolution 100mHz maintained at full range
Features	<ul style="list-style-type: none"> Wide output frequency range: 4, 7, 10, 20MHz Various output waveforms: Sine, Square, and Triangle TTL/CMOS output Variable DC offset control Output overload protection Store/recall: 10 settings Counter up to 150MHz high frequency (SFG-2100 series) AM/FM with internal and external (SFG-2100 series) Sweep mode with LINE and LOG (SFG-2100 series)
Input/Output Terminals	<ul style="list-style-type: none"> Frequency output TTL/CMOS output Counter input (SFG-2100 series) External modulation input (SFG-2100 series)

Front Panel

SFG-2100 series front panel

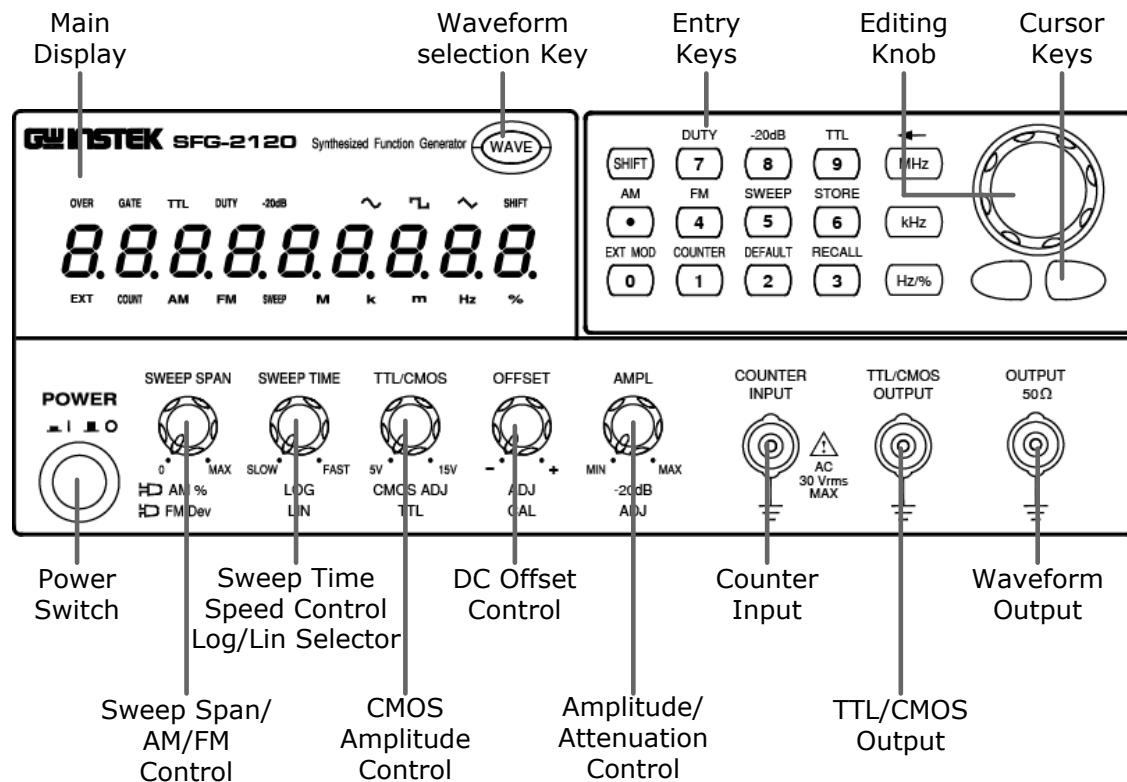

SFG-2000 series front panel

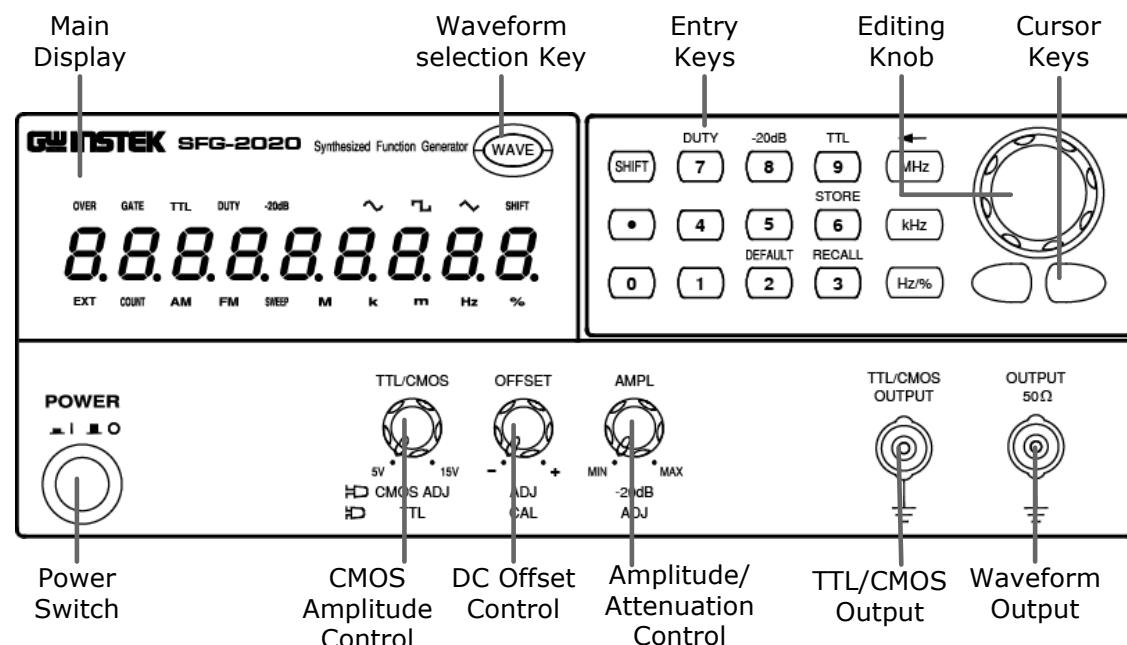

Main display (7 segment)

Shows the waveform frequency, counter frequency, and duty cycle.

OVER

For SFG-2100 series only. In the counter mode, indicates that the leftmost digit (100MHz) is hidden but contains a real number. For counter details, see page40.

GATE

For SFG-2100 series only. In counter mode, indicates gate selection. For counter details, see page40.

TTL

Indicates that the TTL or CMOS output is enabled. For TTL/CMOS details, see page31.

DUTY

For square waveform only.
Indicates that the duty cycle is being edited. For square waveform details, see page25.

-20dB

Indicates that the waveform output is attenuated by -20dB. For attenuation details, see page29.

SWEEP

For SFG-2100 series only. Indicates that the sweep mode is activated. For sweep details, see page35.

FM AM

For SFG-2100 series only. Indicates that FM or AM mode is enabled. For modulation details, see page37 (AM) or page38(FM).

COUNT

For SFG-2100 series only. Indicates that the counter mode is enabled. For counter details, see page40.

EXT

For SFG-2100 series only. Indicates that the external modulation input is used. For details, see page37 (AM) or page39(FM).



Indicates the waveform shape: Sine, Square, and Triangle. For details, see page26.

SHIFT

Indicates that the Shift key is pressed.

M k m Hz

Indicates the output frequency: MHz, kHz, or Hz.

%

Indicates the duty cycle unit. For duty cycle details, see page28.

Waveform selection key



Selects the waveform shape: sine, square, and triangle. For details, see page26.

Entry keys

Enters frequency, duty cycle, and various parameters.

1.2MHz

37kHz

45% (in duty cycle mode)
45Hz (in frequency mode)

Enter duty cycle (page28).

Attenuate the waveform output by -20dB (page29).


Enables TTL/CMOS output (page31).


Deletes previous entry (backspace).

Selects Amplitude Modulation (page37).


Selects Frequency Modulation (page38).

Selects sweep mode (page35).

	STORE 6	Stores the parameter setting (page42).
	RECALL 3	Recalls the parameter setting (page42).
	DEFAULT 2	Recalls the default parameter setting (page43).
	COUNTER 1	Switches to counter mode (page40).
	EXT MOD 0	Accepts external modulation signal (page37-AM) or (page38-FM).
Editing knob		Increases (right turn) or decreases (left turn) the frequency or duty cycle.
Cursor keys		Moves the editing point left or right in case of manual editing.
Waveform output	OUTPUT 50Ω 	Outputs sine, square, and triangle waveform. BNC terminal, 50Ω output impedance.
TTL/CMOS output	TTL/CMOS OUTPUT 	Outputs TTL or CMOS output waveform, BNC terminal. For TTL/CMOS mode details, see page31.
Counter input  Max AC 30Vrms	COUNTER INPUT 	Accepts signals for frequency counting. BNC, AC 30Vrms maximum. For counting mode details, see page40.

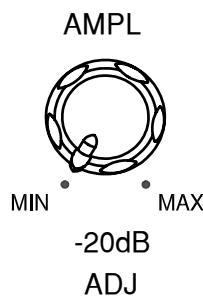
**Amplitude/
Attenuation
control**

Sets the sine/square/triangle waveform amplitude. Turn left (decrease) or right (increase).




When pulled out, attenuates the sine/square/triangle waveform amplitude by -20dB . The -20dB display turns On.

For details, see page29.

**DC offset
control**

When pulled out, sets the DC offset level for sine/square/triangle waveform. Turn left (decrease) or right (increase). The range is $-5\text{V} \sim +5\text{V}$, in 50Ω load.

For details, see page30.

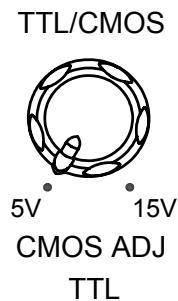**CMOS
amplitude
control**

This knob becomes effective when the TTL/CMOS output is enabled (page31).




Selects TTL as output.



When pulled out, selects CMOS as output. Sets the CMOS output level. Turn left (decrease) or right (increase).

Sweep speed control

SWEEP TIME




This knob is available in SFG-2100 series only. It becomes effective in sweep time mode.

Sets the sweep speed. Turn left (slow) or right (fast). The range is 1 ~ 30 seconds. For sweep details, see page35.




Selects linear sweep.



When pulled out, selects logarithmic sweep.

Sweep span control

SWEEP SPAN




This knob is available in SFG-2100 series only. It becomes effective in sweep mode and AM/FM mode.

In Sweep mode: Sets the sweep span. Turn left (narrow) or right (wide). The range is 1 ~ 100. For sweep details, see page36.

In AM/FM mode:



Sets the FM deviation (page38). Turn left (decrease) or right (increase). The range is over -50kHz ~ +50kHz, centered at 1MHz.




When pulled out, sets the AM depth (page37). Turn left (shallow) or right (deep). The range is 0 ~ 100%.

Power switch

Turns the main power On/Off. For power up sequence, see page20.

Rear Panel

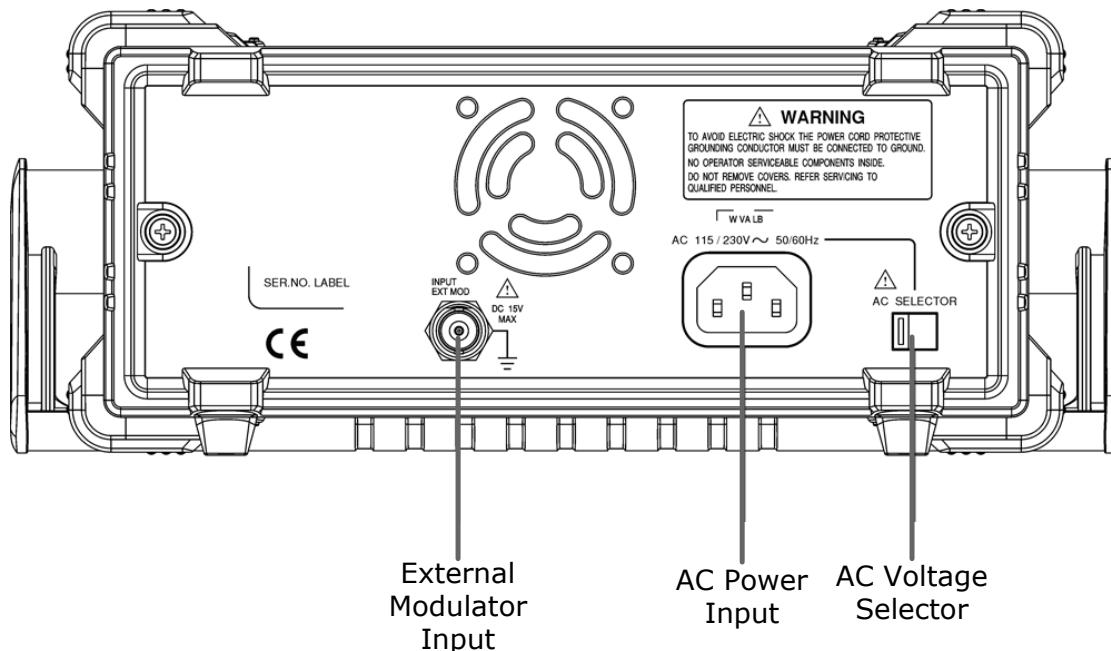

External Modulator Input Accepts the modulation signal from external device. BNC male connector, 10Vp-p maximum. SFG automatically switches the modulation signal from internal to external.
For modulation details, see page37 (AM) or page38(FM).

AC Power Input Accepts the AC power cord. 115 or 230V, 50/60Hz.


AC Voltage Selector Selects 115V or 230V for power source.
AC 100/110/120V → select 115V.

AC 220/230/240V → select 230V.


 Improper selection might lead to internal fuse blowout.

Set Up


Tilt stand

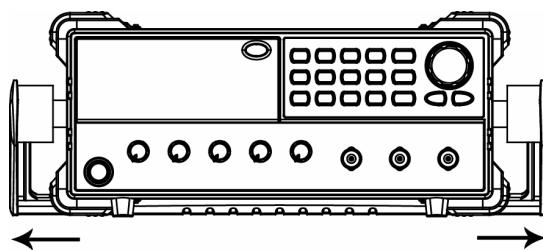


Pull out the handle sideways and rotate it.

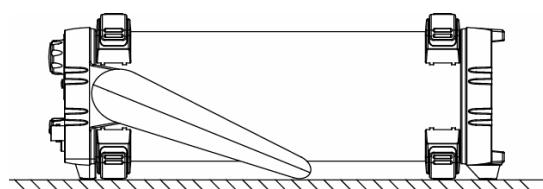

Place SFG horizontally,

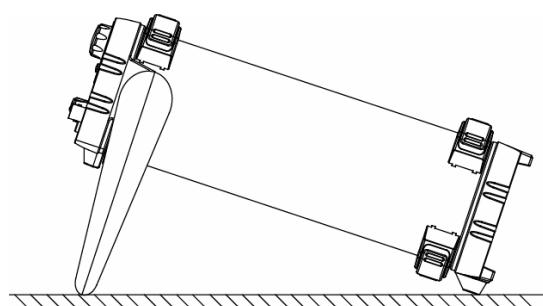

Or tilt stand.

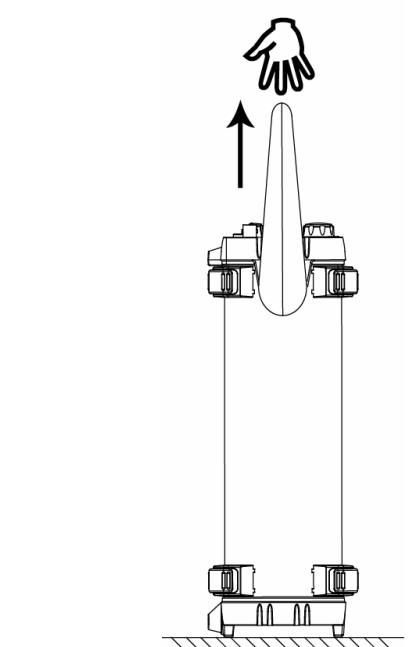


Place the handle vertically for hand carry.

Power up




1. Select the AC voltage on the rear panel accordingly.
AC 100/110/120V → select 115V.
AC 220/230/240V → select 230V.

AC SELECTOR




2. Connect the power cord.



3. Push and turn On the main power switch on the front panel.



4. The display shows model name and the last setup.
Example: SFG-2110, 500Hz triangle wave in sweep mode and -20dB attenuation enabled

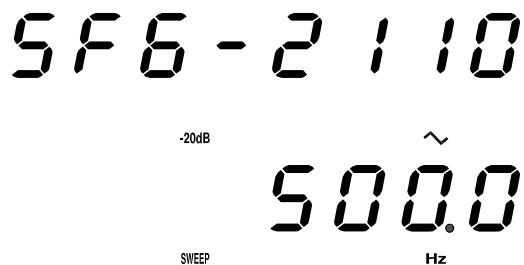


Recall the default setting

Press **SHIFT** **2** **DEFAULT** to recall the default setup. SFG shows the message “done”, and outputs 10kHz sine wave.



Functionality check

Connect SFG output to measurement device such as oscilloscope and check the waveform characteristics.

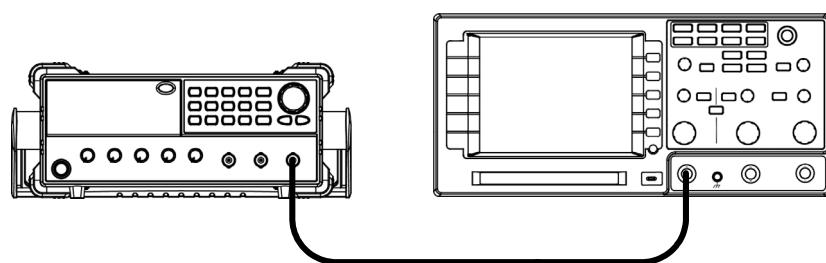

Operation Shortcuts

Here are the collections of operation example shortcuts.

Sine wave 250Hz,
–20dB amplitude

OUTPUT
50Ω



Triangle wave
8kHz,
+2V Offset

OUTPUT
50Ω



Square Wave
1MHz, 45% duty

OUTPUT
50Ω



TTL Output 10kHz

TTL/CMOS
OUTPUT





CMOS Out 10kHz,
10Vpp


TTL/CMOS
OUTPUT




1. Press Wave key and select Sine
2. Press 2 + 5 + 0 + Hz/% key
3. Press Shift + 8 key (-20dB)
...Or pull Amplitude knob



1. Press Wave key and select Triangle
2. Press 8 + kHz key
3. Pull Offset knob (ADJ) and Rotate





1. Press Wave key and select Square
2. Press 1 + MHz key
3. Press Shift + 7 key (Duty)
4. Press 4 + 5 + Hz/% key
...Or Rotate the Scroll knob






or



1. Press Shift + 9 key (TTL)
2. Press 1 + 0 + kHz key
3. Press TTL/CMOS knob (TTL)



1. Press Shift + 9 key (TTL)
2. Press 1 + 0 + kHz key
3. Pull TTL/CMOS knob (CMOS)
and rotate



Linear Sweep,
1kHz start,
Sine wave 250Hz

OUTPUT
50Ω



Log Sweep,
10kHz start,
Triangle wave
8kHz

OUTPUT
50Ω



AM, Internal,
50% modulation,
sine wave 10kHz

OUTPUT
50Ω



FM, External,
50% deviation,
sine wave 1MHz

OUTPUT
50Ω



1. Press Wave key and select Sine
2. Press 2 + 5 + 0 + Hz/% key
3. Press Shift + 5 key (Sweep)
4. Press SWEEP TIME knob (LIN) and rotate
5. Press SWEEP SPAN knob and rotate

1. Press Wave key and select Triangle
2. Press 8 + kHz key
3. Press Shift + 5 key (Sweep)
4. Pull SWEEP TIME knob (LOG) and rotate
5. Press SWEEP SPAN knob and rotate

1. Press Wave key and select Sine
2. Press 1 + 0 + kHz key
3. Press Shift + .(dot) key (AM)
4. Pull SWEEP SPAN knob (AM %) and rotate

1. Press Wave key and select Sine
2. Press 1 + MHz key
3. Input external modulation signal (EXT sign appears)
4. Press Shift + 4 key (FM)
5. Push SWEEP SPAN knob (FM Dev) and rotate

Counter input,
sine wave 1MHz

COUNTER
INPUT



Store the setting
to memory No.1

Recall the setting
from memory
No.1

1. Press Shift + 1 (Counter)

COUNT

2. The Gate sign flashes when counted

GATE

1. Press Shift + 6 (Store)

STORE

6

2. The "Store" sign appears

Store

0

3. Enter the memory number (1 ~ 10)

Store

1

4. The "done" sign appears

done

1. Press Shift + 3 (Recall)

RECALL

3

2. The "Recall" sign appears

RECALL

0

3. Enter the memory number (1 ~ 10)

RECALL

1

4. The "done" sign appears

done

Default Setting Contents

Recall default
settings

SHIFT **2**

Press the shift key, then 2 to recall the default setting. The "done" message appears, followed by display update.

done
10.0000

Wave type	Sine wave
Frequency	10.0000kHz
TTL/CMOS	Disabled
-20dB	Disabled
Modulation	Disabled
Sweep mode	Disabled

SINE/SQUARE/TRIANGLE WAVE



Select waveform	Select the waveform.....	26
Set frequency	Enter frequency.....	26
	Edit frequency.....	27
Set duty cycle	Enter duty cycle	28
(for square wave)	Edit duty cycle.....	28
Set amplitude	Normal output.....	29
	Attenuate by -20dB	29
Set offset	Activate offset.....	30
	Adjust offset	30
	Limitation	30

Select the waveform

Sine / Square
/ Triangle

Press  key repeatedly. The corresponding icon appears on the display.



Sine waveform.



Square waveform.



Triangle waveform.

OUTPUT
50Ω



The waveform comes out from the main terminal.

10Vp-p maximum (50Ω load)

20Vp-p maximum (no load)

Set the Frequency

Enter
frequency

Enter the waveform frequency using the numerical keys.

   MHz

1.2MHz

  kHz

37kHz

  Hz/%

45Hz

 MHz

Delete a number
(backspace)

▲ Triangle waveform frequency is limited to maximum 1MHz. When the input exceeds it, the following message (Freq-Err2) appears and forces the frequency to 1MHz.

FREQ-ERR2

For full error message list, see page52.

Edit
frequency




Left cursor key moves the active cursor left.

(Flashing)
100.0→100.0




Right cursor key moves the active cursor right.

(Flashing)
100.0→100.0



Turn the editing knob left to decrease the frequency.

(Flashing)
100.0→99.0



Turn the editing knob right to increase the frequency.

(Flashing)
100.0→10 10

Set the Duty Cycle (Square Waveform)

The duty cycle setting is not available in sine/triangle waveform.

Enter duty cycle

DUTY
SHIFT 7

Press the Shift key, then 7 to enter duty cycle editing mode. The duty sign appears on the display.



50
%


The default value is 50%.

4 5 Hz/%
SHIFT MHz ←

The settable range is 20% ~ 80%, 2Hz ~ 1MHz.
Use numerical keys to enter value.
Example: 45%

Delete a number (backspace)

Edit duty cycle



The editing knob changes the value, and the cursor keys moves the active digit (same as entering frequency).

When inactive for 5 seconds, the display automatically goes back to previous mode (frequency view).


Setting duty cycle (press SHIFT 7) is not available when sine or triangle waveform is activated. The following message appears.

dut 4 - Err !

For full error message list, see page52.

Set Amplitude

Normal output

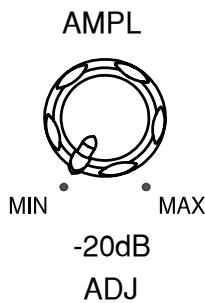


Turn the Amplitude knob right (increase) or left (decrease).

The range is 10Vpp for 50Ω load.

Attenuate by
-20dB

Sine/square/triangle waveform can be attenuated by -20dB, in two ways: -40dB altogether.



Method1

Pull out the Amplitude knob. The output amplitude is attenuated by -20dB (no display sign).




Method2

Press the shift key, then 8. The output amplitude is attenuated by -20dB. The -20dB sign appears on the display.


Set Offset

Activate offset

SFG can add or delete offset to the sine/square/triangle waveform, thus changing the waveform vertical position. Use the OFFSET knob.




Pushed: Offset Off



Pulled: Offset On

Adjust offset



Turn the knob right (higher position) or left (lower position).

The range is $-5V \sim +5V$ for 50Ω load.

Limitation




Note that the output amplitude, including the offset, is still limited to:

$-5 \sim +5V$ (50Ω load)


$-10 \sim +10V$ (no load)

Therefore excessive offset leads to peak clip as below.

Positive peak clip (50Ω)

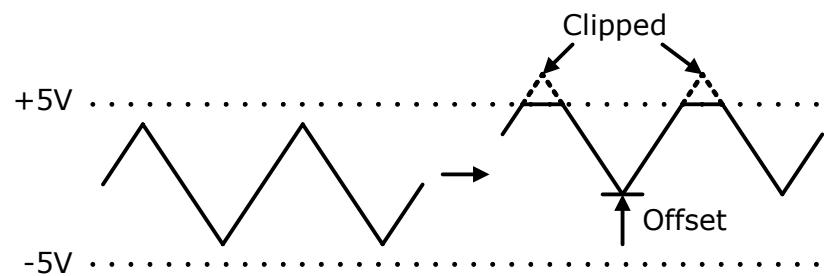

Negative peak clip (50Ω)

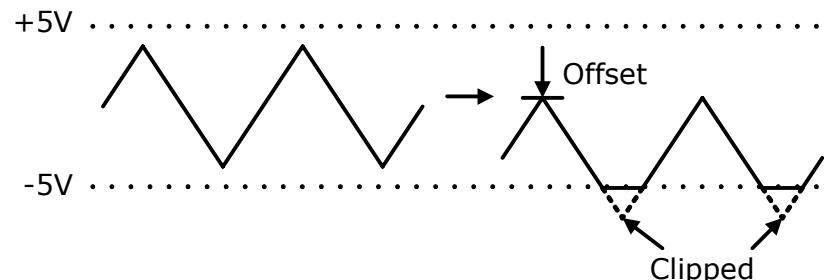

TTL CMOS OUTPUT



Select waveform	Select the waveform.....	32
Set frequency	Enter frequency.....	32
	Edit frequency.....	33
Set duty cycle	Enter duty cycle	33
	Edit duty cycle.....	34
Set amplitude	Set Amplitude.....	34

Select the waveform

TTL/CMOS




Press Shift key, then 9. The TTL sign appears on the display.


TTL

The TTL/CMOS output is always On when the square wave is activated.


TTL/CMOS



Push/pull the TTL/CMOS knob to select the waveform.



Pushed: TTL is selected as output.



Pulled: CMOS is selected as output.

TTL/CMOS
OUTPUT

The waveform comes out from the TTL/CMOS terminal.

TTL: $\geq 3\text{Vp-p}$ (fixed)

CMOS: $4\text{V}\pm 1\text{Vp-p} \sim 15\pm 1\text{Vp-p}$


Set the Frequency

Enter frequency


Enter the waveform frequency using the numerical keys.



1.2MHz



37kHz



45Hz



Delete a number
(backspace)

Edit frequency




Left cursor key moves the active cursor left.

(Flashing)
100.0 → 100.0




Right cursor key moves the active cursor right.

(Flashing)
100.0 → 100.0



Turn the editing knob left to decrease the frequency.

(Flashing)
100.0 → 99.0



Turn the editing knob right to increase the frequency.

(Flashing)
100.0 → 10 10

Set the Duty Cycle

Enter duty cycle

SHIFT 7 DUTY

Press the Shift key, then 7 to enter duty cycle editing mode. The duty sign appears on the display.

50
%

4 5 Hz/%

SHIFT MHz ←


The default value is 50%.

The settable range is 20% ~ 80%, 2Hz ~ 1MHz.

Use the numerical keys to enter value. Example: 45%

Delete a number (backspace)

Edit duty cycle




The editing knob changes the value, and the cursor keys moves the active digit (same as entering frequency).

When inactive for 5 seconds, the display automatically goes back to previous mode (frequency view).

Set Amplitude

CMOS waveform


TTL/CMOS



Use the TTL/CMOS knob.



Pushed: selects TTL output with fixed amplitude, min. 3Vp-p.



Pulled: selects CMOS output, amplitude range $4V \pm 1V$ p-p ~ $15 \pm 0.5V$ p-p.

Turn the knob right (increase amplitude) or left (decrease amplitude).

SWEET

SFG can add sweep to the waveform output, a convenient tool for measuring the frequency response of the DUT.



- Sweep function applies only to SFG-2100 series.
- Sweep and Modulation (page37) cannot be used together.

**Activate
sweep**

1. Output the waveform. Sine/Triangle/Square (page25) or TTL/CMOS (page31).
2. Press the Shift key, then 5 (Sweep).




3. Sweep is activated and the sign appears on the display.

SWEET



When the sweep is activated, the duty cycle of Square/TTL/CMOS wave is fixed to 50%.

**Select
Log/Lin
Sweep**



Logarithmic Sweep:

Pull the SWEEP TIME knob.



Linear Sweep:


Push the SWEEP TIME knob.



Set Sweep Time

Sweep time sets the time it takes for a single sweep from the start frequency to the end frequency.

Rotate the SWEEP TIME knob, right (fast) or left (slow).



Range 1 ~ 30 seconds




Note: If the sweep time becomes too long, the stop frequency might reach the rating (4, 7, 10, or 20MHz). In this case, the frequency stays at the rating to the end.

Set Sweep Span

Sweep span sets the frequency width of the sweep.

The current output frequency becomes the start frequency.

Rotate the SWEEP SPAN knob, right (wide) or left (narrow).



Range 1 ~ 100 frequency ratio



Note: In order to get the maximum span (frequency ratio), set the sweep time to a sufficient length (not too short).

AMPLITUDE MODULATION




- AM applies only to SFG-2100 series.
- Modulation and Sweep (page35) cannot be used together.

Activate AM

1. Output the waveform, Sine/Triangle/Square (page25).
2. Press the Shift key, then Dot (AM). AM is activated and the sign appears on the display.

AM
SHIFT ● **AM**


Set AM depth

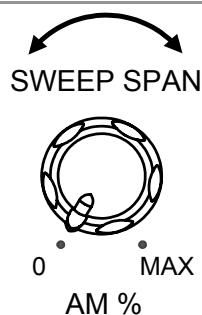

1. Pull the SWEEP SPAN knob (AM %).
2. Turn the knob left (shallow) or right (deep).

Range $0 \sim 100\%$

Use external modulating signal



SFG-2000 series uses an internal 400Hz sine wave as the default modulating signal.

1. Connect the modulating signal to the rear panel terminal.
2. Press the Shift key, then 0 (EXT MOD). External modulation is activated.

EXT MOD
SHIFT 0 **EXT**

Frequency Range DC ~ 1MHz

FREQUENCY MODULATION



- FM applies only to SFG-2100 series.
- Modulation and Sweep (page35) cannot be used together.

Activate FM

1. Output the waveform. Sine/Triangle/Square (page25) or TTL/CMOS (page31).
2. Press the Shift key, then 4 (FM). FM is activated and the sign appears on the display.

SHIFT **4** **FM**




When FM is activated, the duty cycle of Square/TTL/CMOS wave is fixed to 50%.

Set FM deviation

The output frequency becomes the Center Frequency.

SWEEP SPAN



1. Push the SWEEP SPAN knob (FM Dev).



2. Turn the knob left (shallow) or right (deep).

Deviation

0 ~ ±50kHz, centered at 1MHz

Range



When the deviation is added to the center frequency, the result must be smaller than the rating frequency.

**Center Frequency + Deviation \leq
Rating(4,7,10,20MHz)**

When this rule is violated, the “Freq-Err3” error message appears and the FM setting will be cancelled.

F F E 9 - E R R 3

For more error message details, see page52.

Center frequency (=Output frequency) must be set within this range.


SFG-2104 300kHz ~ 3.7MHz

SFG-2107 300kHz ~ 6.7MHz

SFG-2110 300kHz ~ 9.7MHz

SFG-2120 300kHz ~ 19.7MHz

Use external modulating signal



SFG-2000 series uses an internal 400Hz sine wave as the default modulating signal.

1. Connect the modulating signal to the rear panel terminal.
2. Press the Shift key, then 0 (EXT MOD). External modulation is activated.

SHIFT 0 EXT MOD EXT

Frequency	1kHz (fixed)
Range	

COUNTER INPUT



Counter input applies only to SFG-2100 series.

**Activate
counter**

COUNTER
INPUT



1. Connect the signal input to the Counter input terminal. Press Shift key, then 1 (Counter).
2. EXT and COUNT sign appear on the display.

EXT COUNT

3. The display shows the input signal frequency.

GATE ~
3 17386
k Hz
EXT COUNT

4. The GATE sign flashes when the gate condition is met.

GATE

Range 0 ~ 150MHz


Resolution 100nHz for 1Hz input,
0.1Hz for 100MHz input

**Set the gate
time**

Gate time sets the display update rate and counter resolution. These two parameters are in trade-off.

Short gate time = faster update, coarse resolution

Long gate time = slower update, fine resolution



To change the gate time, turn the editing knob right (increase) or left (decrease).

Gate time / Resolution table

The following table shows the relationship between counter frequency, gate time, resolution, and display.

	Input	Gate time	Resolution	Display
1Hz		0.01s	100µHz	1.0000Hz
		0.1s	10µHz	1.00000Hz
		1s	1µHz	1.000000Hz
		10s	100nHz	1.0000000Hz
10Hz		0.01s	100µHz	10.0000Hz
		0.1s	10µHz	10.00000Hz
		1s	1µHz	10.000000Hz
		10s	100nHz	10.0000000Hz
100Hz		0.01s	1mHz	100.000Hz
		0.1s	100µHz	100.0000Hz
		1s	10µHz	100.00000Hz
		10s	1µHz	100.000000Hz
1kHz		0.01s	10mHz	1.00000kHz
		0.1s	1mHz	1.000000kHz
		1s	100µHz	1.0000000kHz
		10s	10µHz	1.00000000kHz
1MHz		0.01s	10Hz	1.00000MHz
		0.1s	1Hz	1.000000MHz
		1s	100mHz	1.0000000MHz
		10s	10mHz	1.00000000MHz
10MHz		0.01s	100Hz	10.0000MHz
		0.1s	10Hz	10.00000MHz
		1s	1Hz	10.000000MHz
		10s	100mHz	10.0000000MHz
100MHz		0.01s	100Hz	100.0000MHz
		0.1s	10Hz	100.00000MHz
		1s	1Hz	100.000000MHz
		10s	100mHz	00.0000000MHz*

Over sign

* The OVER sign shows that the 100MHz digit contains a real number but hidden from the display. It turns On under the following condition.

OVER

- Input frequency: $\geq 100\text{MHz}$
- Gate Time: 10s

To view the 100MHz digit, switch to smaller gate time such as 1s or 0.1s.

STORE/RECALL SETTING



Store the panel setting

SHIFT **STORE
6**

Press the Shift key, then 6 to store the current panel setting to internal memories.

Memory range: 0 ~ 9 (10 set)

The “Store 0” sign appears.

StorE 0

Enter the memory number, 0 ~ 9. (for example, 1)

StorE 1

The “done” sign appears.

done

Recall the panel setting

SHIFT **RECALL
3**

Press the Shift key, then 3 to recall a panel setting stored in internal memories.

Memory range: 0 ~ 9 (10 set)

The “recall 0” sign appears.

Recall 0

Enter the memory number, 0 ~ 9. (for example, 1)

Recall 1

The “done” sign appears and the panel setting changes accordingly.

done

Recall the default panel setting

SHIFT **DEFAULT**
 2

Press the shift key, then 2 to recall the default panel setting.

The “done” message appears.

done

The panel is updated with the default setting.


~
10.0000
k Hz

Wave type	Sine wave
Frequency	10.0000kHz
TTL/CMOS	Disabled
-20dB	Disabled
Modulation	Disabled
Sweep mode	Disabled

APPLICATION EXAMPLES


Reference Signal for PLL System

Description	The SFG output can be used as a cost-effective reference signal for Phase-Locked-Loop system. Directly connect SFG output to PLL input.
--------------------	---

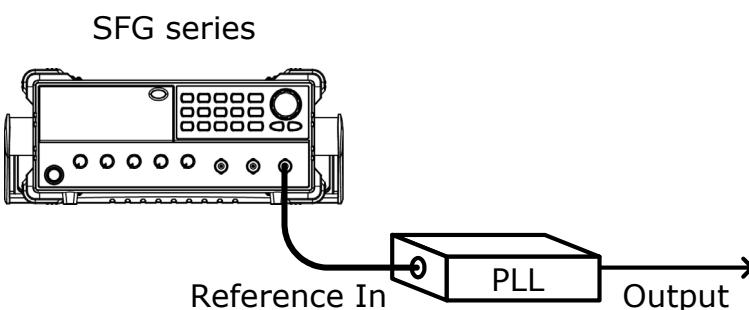Block diagram

Trouble-Shooting Signal Source

Description	The SFG output can be used as the signal source to test the failed part in a circuit system. Isolate the problematic part from the rest, feed the SFG output as a stimulus, and observe the outcome using an oscilloscope.
--------------------	--

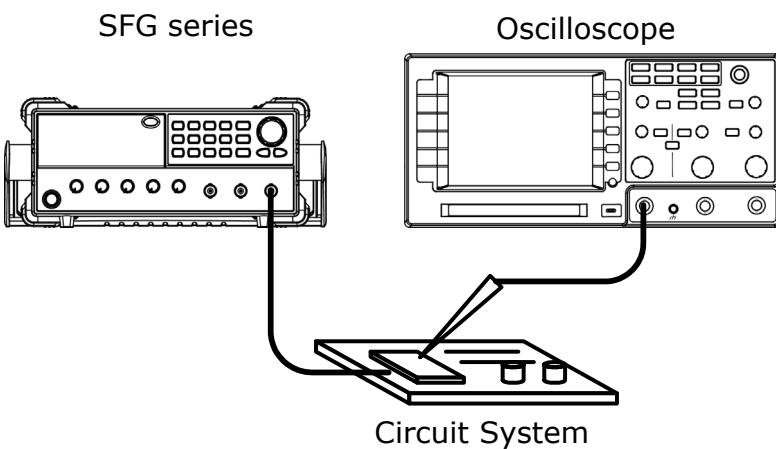
Block diagram

Transistor DC Bias Characteristics Test


Description

Use SFG-2000 series as the signal source for a transistor. Compare the transistor input/output waveform using the oscilloscope. Adjust the DC voltage source to find out the maximum output without distorting the waveform.

Block diagram

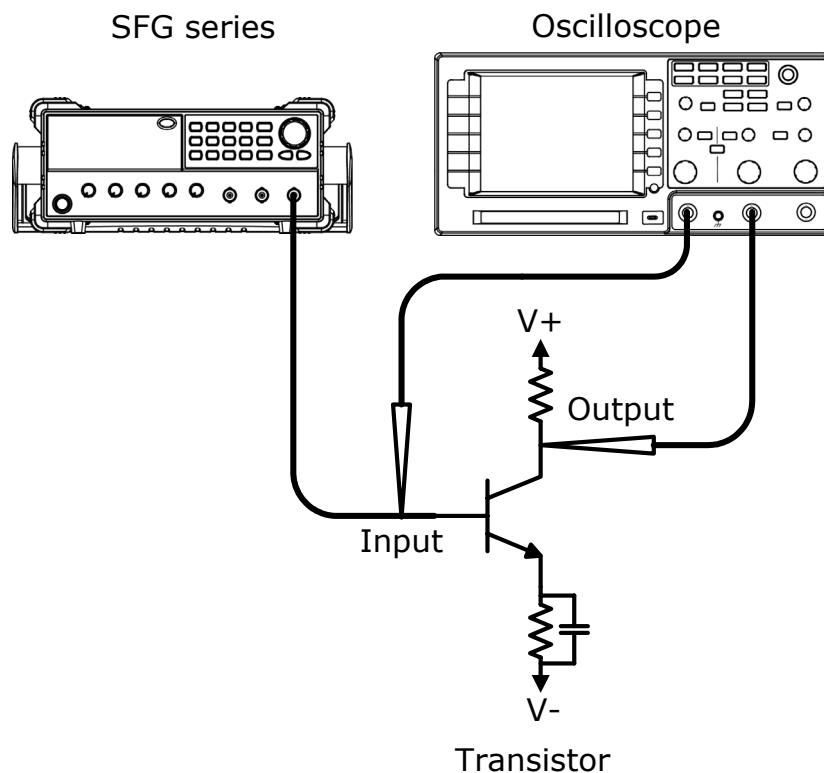

Oscilloscope display

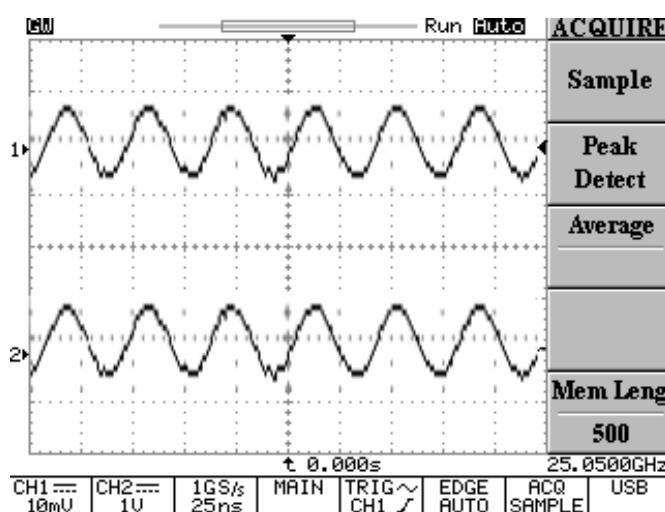


Amplifier Over-Load Characteristic Test

Description

Use the triangle wave output from SFG-2000 series to check the amplifier output distortion caused by overload. The common sine wave is not the ideal source in this case. Observe the linearity of the triangle waveform using an oscilloscope.

Block diagram

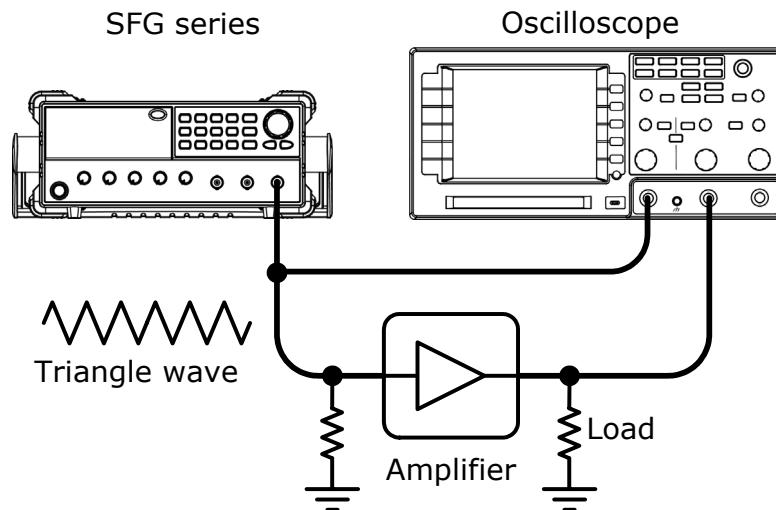


Amplifier Transient Characteristics Test

Description

Use the square wave output from SFG-2000 series to check the transient frequency response of an amplifier. The common sine wave is not the ideal source in this case. Observe the waveform using an oscilloscope.

Block diagram

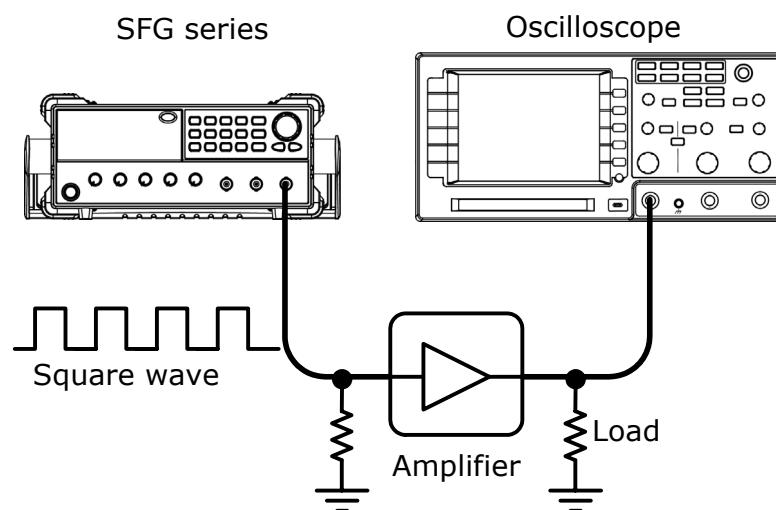

Test step

1. Apply a triangle waveform to the amplifier first.
Adjust the waveform amplitude to make sure there is no clipping.
2. Switch to square waveform and adjust its frequency to the middle of the amplifier pass band, such as 20Hz, 1kHz, and 10kHz.
3. Observe the shape of the amplifier output. The following table shows the possible output distortions and their explanations.

Transient characteristic list

- Amplitude reduction at low frequency
- No phase shift




- Low frequency boosted (accentuated fundamental)



- High frequency loss
- No phase shift



- Low frequency phase shift
- Trace thickened by hum-voltage



- High frequency loss
- Phase shift



- Low frequency loss
- Phase shift



- Low frequency loss
- Low frequency phase shift



- High frequency loss
- Low frequency phase shift



- Damped oscillation


**Note**

For narrow band amplifier testing, square wave may not be suitable.

Logic Circuit Test

Description


Use the TTL/CMOS output from SFG-2000 series to test digital circuits. Observe the timing relation of input/output waveform using an oscilloscope.

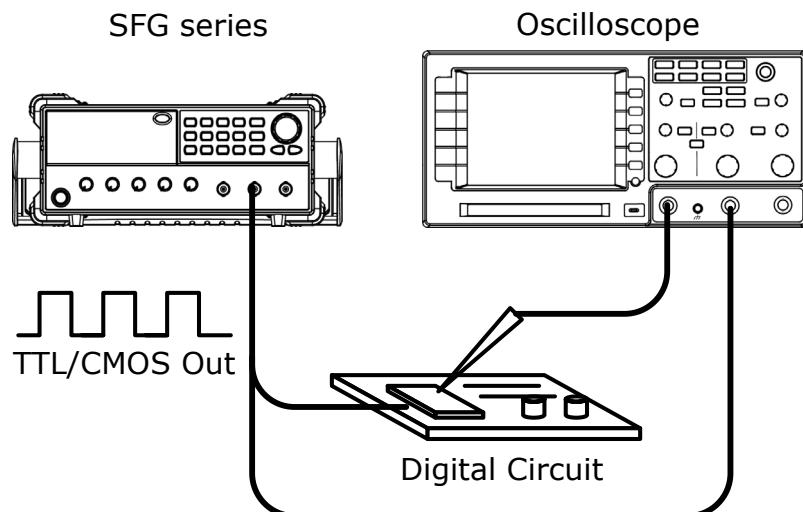Block diagram


Impedance Matching Network Test

Description


Use SFG-2000 series for impedance matching network: testing its frequency characteristic and matching the impedance.

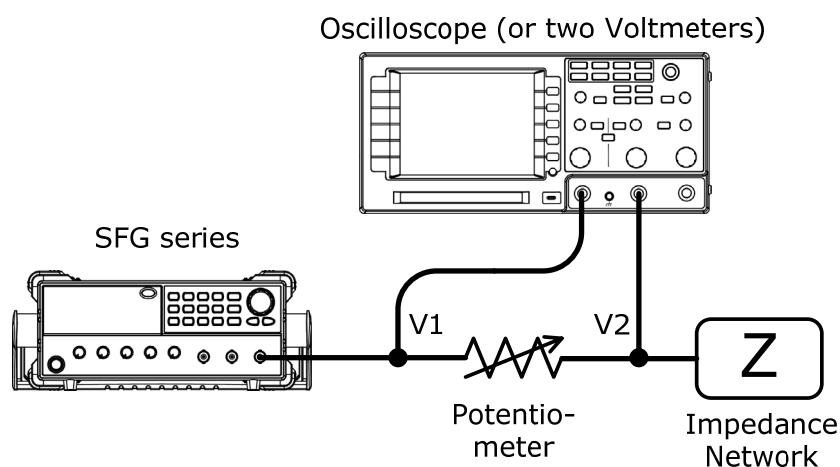Block diagram

Test step


Adjust the potentiometer until V2 becomes the half of V1 ($V_2=0.5V_1$). Then the impedance Z of the network becomes identical to the potentiometer.

Speaker Driver Test

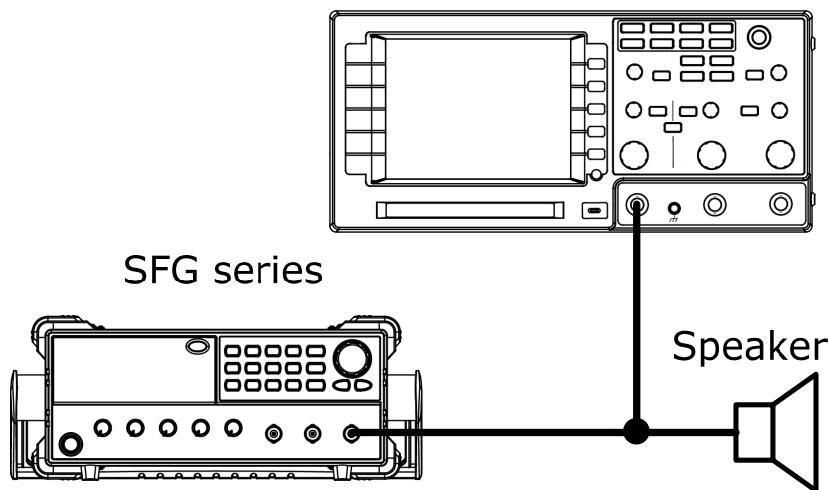Description	Use SFG-2000 series for testing the frequency characteristics of audio speakers. Record the volt reading versus the input signal frequency.
--------------------	---

Block diagram**Oscilloscope (or Voltmeter)****Graph**

The peak voltage occurs on the resonant frequency of the speaker.

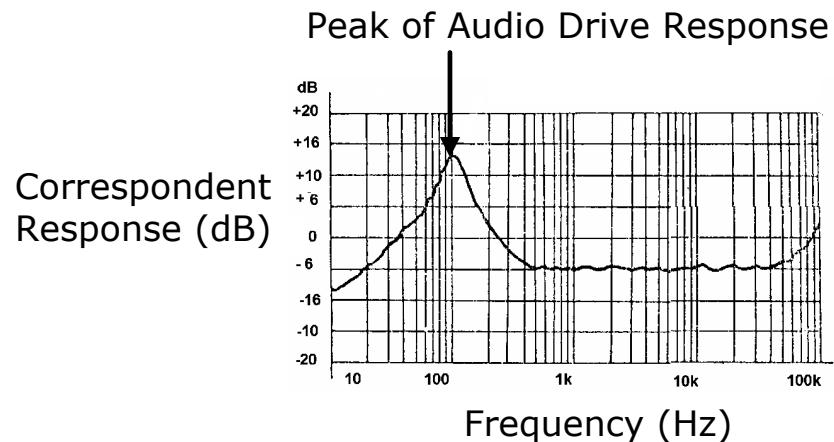


Sweep for Speaker Test

Description Use the sweep feature in SFG-2000 series for testing the frequency response of an audio speaker.

- Test description**
1. Set SFG output to sine wave, 20Hz.
 2. Activate sweep and set LIN/LOG, sweep time, and sweep span.
 3. Change the frequency if other bands need to be tested.
-

Block diagram

SFG series

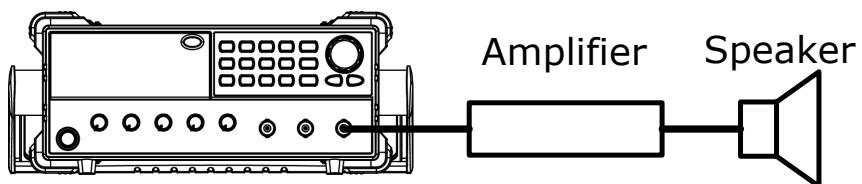

FAQ

-
- I pressed the Power key on the front panel but nothing happens.
 - How can I get out of Counter/Sweep/Modulation/TTL/-20dB mode?
 - The device accuracy does not match the specification.
 - What are these error messages?
-

I pressed the Power key on the front panel but nothing happens.

Make sure the AC source voltage setting on the rear panel is correct (page21). Otherwise the internal fuse might be blown out. Contact the service personnel.

How can I get out of Counter/Sweep/Modulation/TTL/-20dB mode?

Press the Shift key, then the relevant numerical key. (Do the same action as you entered those modes)

For example: To get out of Counter mode, press Shift then 1.

The device accuracy does not match the specification.

Make sure the device is powered On for at least 30 minutes, within +20°C~+30°C. This is necessary to stabilize the unit to match the specification.

What are these error messages?

Several messages appear when trying to set the frequency or duty cycle in forbidden way. Page52 summarizes all the error message content.

If there is still a problem, please contact your local dealer or GWInsteak at www.gwinstek.com.tw / marketing@goodwill.com.tw.

APPENDIX

Error Messages

Frequency
error

F F E 9 - E R R

FrEq-Err1	Sine and square wave frequency over range. This message appears when entering sine or square waveform frequency larger than the rating. See page26 for sine/square rating.
FrEq-Err2	Triangle wave Frequency over range. This message appears when entering triangle waveform frequency larger than 1MHz. See page26 for triangle wave rating.
FrEq-Err3	FM Center Frequency over range. This message appears when trying to enter FM center frequency larger than specified. See page38 for FM center frequency range.

Duty Cycle
error

d u t y - E R R

duty-Err1	Not square waveform. This message appears when trying to set duty cycle in non-square (=sine or triangle) waveform. For duty cycle setting, see page28 (square wave) or page33 (TTL/CMOS output).
duty-Err2	Square wave frequency over range. This message appears when trying to set duty cycle when the square wave frequency is over 1MHz. For square wave frequency setting, see page26.
duty-Err3	Duty over range. This message appears when the duty cycle setting goes outside 20~80% range. For duty cycle range, see page28 (square wave) or page33 (TTL/CMOS output).

Specification

Main	Output Function	Sine, Square, Triangle
	Amplitude Range	10Vp-p (into 50Ω load)
	Impedance	50Ω ± 10%
	Attenuator	-20dB ± 1dB x2
	DC Offset	< -5V ~ >+5V (50Ω load)
	Duty Range	20% ~ 80%, 2Hz~1MHz (Square Wave)
	Duty Resolution	1% (Square Wave Only)
Frequency	Display	9 digits LED display
	Sine/Square Waveform Range	SFG-2004 0.1Hz ~ 4MHz SFG-2007 0.1Hz ~ 7MHz SFG-2010 0.1Hz ~ 10MHz SFG-2020 1Hz ~ 20MHz SFG-2104 0.1Hz ~ 4MHz SFG-2107 0.1Hz ~ 7MHz SFG-2110 0.1Hz ~ 10MHz SFG-2120 1Hz ~ 20MHz
	Triangle Waveform Range	0.1Hz ~ 1MHz (1Hz ~ 1MHz for SFG-2020/2120)
	Resolution	0.1Hz (1Hz for SFG-2020/2120)
	Stability	±20ppm
	Accuracy	±20ppm
	Aging	±5ppm/year
	Harmonic Distortion	≥-55dBc, 0.1Hz ~ 200kHz ≥-40dBc, 0.2MHz ~ 4MHz ≥-30dBc, 4MHz ~ 20MHz (Amplitude at maximum position without attenuating 1/10 of any combination setting, TTL/CMOS off)
	Flatness	< ± 0.3dB, 0.1Hz ~ 1MHz < ± 0.5dB, 1MHz ~ 4MHz < ± 2dB, 4MHz ~ 10MHz < ± 3dB, 10MHz ~ 20MHz (At the max amplitude relating to 1kHz)
Triangle Wave	Linearity	≥ 98%, 0.1Hz ~ 100kHz ≥ 95%, 100kHz ~ 1MHz
Square Wave	Symmetry	±1% of period + 4ns, 0.1Hz ~ 100kHz
	Rise/Fall Time	≤ 25ns at maximum output (50Ω load)
CMOS Output	Level	4 ± 1Vpp ~ 15 ± 1Vpp, adjustable
	Rise/Fall Time	≤ 120ns

TTL Output	Level	$\geq 3\text{Vpp}$
	Fan Out	20 TTL Load
	Rise/Fall Time	$\leq 25\text{ns}$
Sweep (SFG-2100 Series)	Sweep Rate	100:1 Ratio Max, adjustable (Note1)
	Sweep Time	1 ~ 30s, adjustable (Note2)
	Sweep Mode	Linear, Logarithmic
Amplitude Modulation (SFG-2100 Series)	Depth	0 ~ 100%
	Frequency	400Hz (internal), DC ~ 1MHz (external)
	Carrier BW	100Hz ~ 5MHz (-3dB)
Frequency Modulation (SFG-2100 Series)	External Modulating	Sensitivity: $\leq 10\text{Vpp}$ for 100% modulation
	Deviation	$\geq 0 \sim \pm 50\text{kHz}$, center at 1MHz
	Frequency	400Hz fixed (internal), 1kHz fixed (external)
Frequency Counter (SFG-2100 Series)	External Modulating	Sensitivity: $\leq 10\text{Vpp}$ for 10% modulation (center at 1MHz)
	Range	5Hz ~ 150MHz
	Accuracy	Time Base Accuracy ± 1 count
Store/Recall	Time Base	$\pm 20\text{ppm}$ ($23 \pm 5^\circ\text{C}$) after 30min warmup
	Max. Resolution	100nHz for 1Hz, 0.1Hz for 100MHz
	Input Impedance	$1\text{M}\Omega/150\text{pf}$
General	Sensitivity	$\leq 35\text{mVrms}$, 5Hz ~ 100MHz $\leq 45\text{mVrms}$, 100MHz ~ 150MHz
	Power Source	AC115V/230V +10%, -15%, 50/60Hz Indoor Use, Altitude Up to 2000m
	Operation Environment	Ambient Temperature 0 ~ 40°C Relative Humidity $\leq 80\%$, 0 ~ 40°C Relative Humidity $\leq 70\%$, 35 ~ 40°C Install Category II / Pollution Degree 2
General	Storage Environment	Temperature: -10 ~ 70°C Humidity: $\leq 70\%$
	Accessories	Instruction Manual x 1, Power Cord x 1 GTL-101 x 2 (SFG-2100 Series) GTL-101 x 1 (SFG-2000 Series)
	Dimension	107 (W) x 266 (H) x 293 (D)
General	Weight	Approx. 3.2kg (SFG-2100 Series) Approx. 3.1kg (SFG-2000 Series)

Note1: In order to get the maximum sweep span, sweep time needs to be tuned.

Note2: If sweep time is too long, the stop frequency will stay at the maximum frequency until the end of the sweep cycle.

Declaration of Conformity

We

GOOD WILL INSTRUMENT CO., LTD.

(1) No.7-1, Jhongsing Rd., Tucheng City, Taipei County, Taiwan

(2) No. 69, Lu San Road, Suzhou City (Xin Qu), Jiangsu Sheng, China
declare, that the below mentioned product

Type of Product: Synthesized Function Generator

**Model Number: SFG-2004, SFG-2007, SFG-2010, SFG-2020,
SFG-2104, SFG-2107, SFG-2110, SFG-2120**

are herewith confirmed to comply with the requirements set out in the Council Directive on the Approximation of the Law of Member States relating to Electromagnetic Compatibility (89/336/EEC, 92/31/EEC, 93/68/EEC) and Low Voltage Directive (73/23/EEC, 93/68/EEC).

For the evaluation regarding the Electromagnetic Compatibility and Low Voltage Directive, the following standards were applied:

◎ EMC

EN 61326-1: Electrical equipment for measurement, control and laboratory use — EMC requirements (1997 + A1:1998 + A2:2001 + A3:2003)	
Conducted Emission Radiated Emission EN 55011: Class A 1998 + A1:1999 + A2:2002	Electrostatic Discharge EN 61000-4-2: 1995 + A1:1998 + A2:2001
Current Harmonics EN 61000-3-2: 2000 + A2:2005	Radiated Immunity EN 61000-4-3: 2002 + A1:2002
Voltage Fluctuations EN 61000-3-3: 1995 + A1:2001	Electrical Fast Transients EN 61000-4-4: 2004
-----	Surge Immunity EN 61000-4-5: 1995 + A1:2001
-----	Conducted Susceptibility EN 61000-4-6: 1996 + A1:2001
-----	Power Frequency Magnetic Field EN 61000-4-8: 1993 + A1:2001
-----	Voltage Dip/ Interruption EN 61000-4-11: 2004

INDEX

2	setup.....28
20dB attenuation	29
example setting.....	22
 A	
AM	
example setting.....	23
setup	37
amplifier application example.....	46
application examples	44
 C	
cleaning.....	7
CMOS	
activation.....	32
example setting.....	22
constant current circuit	10
control knob overview	17
counter gate time	40
counter input	40
example setting.....	24
 D	
DDS block diagram	11
default panel setting	
contents	43
recall	43
default setting	
contents	24
default setting recall.....	21
direct digital synthesis	10
display contents overview.....	14
duty cycle	
example setting.....	22
 E	
EN 61010.....	6, 7, 55
EN55011.....	55
EN61000.....	55
external modulation	37, 39
example setting	23
 F	
FAQ.....	51
FM	
example setting	23
seup	38
frequency	
editing	27
entering.....	26
frequency error	27, 39, 52
faq.....	51
front panel diagram	
SFG-2000	13
SFG-2100	13
fuse	
safety instruction	6
 I	
impedance application example.....	48
in/out terminal overview	16
 L	
lin sweep selection	35
log sweep selection.....	35
logic application example.....	48

M

main feature list.....12

memory recall

example setting.....24

memory store

example setting.....24

model lineup.....12

N

numerical keys overview15

O

offset30

example setting.....22

operation environment

safety instruction.....7

operation shortcuts22

P

phase locked loop

example application.....44

power supply

safety instruction.....6

power up sequence21

FAQ.....51

R

rear panel19

recall setting.....42

S

safety

guidelines6

symbol.....5

UK power cord.....8

setup step.....20

sine wave

example setting22

selection26

speaker application example49, 50

specification53

FAQ51

square wave

duty cycle28

example setting22

selection26

storage environment

safety instruction7

store setting42

sweep

example setting23

setup35

T

table of contents3

technical background10

tilt stand.....20

transistor application example.....45

triangle wave

example setting22

selection26

troubleshooting application example44

TTL

activation32

example setting22