

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

3-348-802-03
8/11.01

- Clear-cut operating menus
- Illuminated display
- Two 4 m measurement cables (4-wire connection)
- Remote control for efficient use
- Limit value adjustment
- Convenient memory and report generating functions
- Data interfaces for PC and printer
- Can be expanded for quick, on-site alphanumeric data entry and reports printing
- Can be retrofitted for high-voltage testing



QUALITY MANAGEMENT SYSTEM



DQS Certified per
DIN EN ISO 9001 reg. no. 1262



Applications

The PROFITEST 204 tester has been designed for quick, safe testing of electrical and electronic equipment and systems at machinery in accordance with DIN EN 60204-1 and VDE 0113 with nominal voltages of up to 1000 V.

The following periodic tests must be performed in accordance with the standard:

- Testing for continuity at connections within the protective conductor system with 10 A test current
- Insulation resistance test
- Voltage tests (*optionally HP or HV*)
- Testing for residual voltage

Beyond this, the following tests and measurements may be performed as well:

- Leakage current test
- Voltage measurement
- Frequency measurement

All values required for approval reports can be measured with this instrument.

Display

The LCD window consists of an illuminated dot matrix display at which menus, device settings and measurement results, as well as online help can be displayed.

Help Key

Information regarding the current menu item can be queried with this key. Online help texts appears at the LCD window.

Function Selector Switch

Testing, report generating and data management functions are selected with the rotary switch.

Limit Values

Limit values can be assigned for use with each measurement, allowing for individualized adaptation of the various tests to prevailing local conditions, as well as to the latest requirements set forth in the standards.

Data Memory

Depending upon the number of systems for which data logging is performed (max. 254), up to 2800 measurements can be saved to memory.

Remote Control

The test probe with integrated control panel allows for remote control of protective conductor and insulation resistance measurements, as well as storage of the respective values to memory. Integrated lamps indicate measurement progress status. All PROFITEST 204 operating functions can also be controlled via the RS 232 interface. Signal and display values can be remote queried as well.

RS 232 Interface for Printer and PC

This port provides for data transmission and the supply of electrical power to the optionally available SECUTEST PSI printer. Other devices (e.g. a PC) can also be connected to this port with the help of an interface cable.

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

CENTRONICS Parallel Port

Any commercially available printer can be connected to this data interface (except for PostScript printers). Detailed report forms which have been uploaded to the instrument can be read out via this port.

Report Generating Functions

The following report generating functions are available:

- Read out measurement data to the integrated SECUTEST PSI printer (accessory)
- Upload report forms to the test instrument with the help of a PC and included PROTOCOL software
- Select one of three report forms stored to the instrument
- Read out measurement data via the CENTRONICS parallel port to commercially available printers
- Transmit measurement data to a PC and process with EXCEL

Characteristic Values

Meas. Quantity	Measuring Range	Nominal Range of Use	Resolution	Nom. Voltage U_N	Open-Circuit Voltage U_0	Nom. Current I_N	Short-Circuit Current I_K	Int. Resist. R_I	Meas. Error	Intrinsic Error	Overload		
											Capacity	Duration	
Protective Conductor Resistance R_{SL}	0 ... 85 m Ω	10 ... 330 m Ω	100 $\mu\Omega$	—	12 V ~	10 A	12 A	—	$\pm(8.6\% \text{ rdg.} + 6 \text{ d})$	$\pm(3\% \text{ rdg.} + 5 \text{ d})$	Fuse: 16 A/1000 V Breaking Capacity: 5 kA		
	85 ... 999 m Ω		1 m Ω										
	1.00 ... 9.99 Ω	—	10 m Ω		12 V ~	—	—		$\pm(3\% \text{ rdg.} + 10 \text{ d})$				
	10.0 ... 25.0 Ω		100 m Ω										
ΔU^*	0 ... 9.99 V*	—	0.01 V	—	12 V ~	10 A	12 A	—	—	$\pm(2\% \text{ rdg.} + 3 \text{ d})$			
	10.0 ... 12.0 V		0.1 V		12 V ~	—	—			$\pm(10\% \text{ rdg.} + 3 \text{ d})$			
Insulation Resistance R_{ISO}	0 ... 999 k Ω	0.050 ... 50 M Ω	1 k Ω	100/250/500/1000 V	max. $1.3 \cdot U_N$	1 mA	max. 1.6 mA	—	$\pm(5.5\% \text{ rdg.} + 4 \text{ d})$ of 0.05M Ω ...50M Ω	$\pm(3\% \text{ rdg.} + 2 \text{ d})$	1200 V	cont.	
	1.00 ... 9.99 M Ω		10 k Ω										
	10.0 ... 99.9 M Ω		100 k Ω										
	100 ... 499 M Ω	—	1 M Ω						250 V	—			$\pm(8\% \text{ rdg.} + 2 \text{ d})$
	500 ... 999 M Ω		1 M Ω						500/1000 V				$\pm(5\% \text{ rdg.} + 2 \text{ d})$
	1 ... 3 G Ω		10 M Ω						1000 V				$\pm(10\% \text{ rdg.} + 2 \text{ d})$
Leakage Current ΔI	0.00 ... 9.99 mA	0.2 ... 9.9 mA	0.01 mA	—	—	—	—	2 k Ω	$\pm(8.6\% \text{ rdg.} + 9 \text{ d})$	$\pm(5\% \text{ rdg.} + 5 \text{ d})$	250 V	cont.	
Voltage $U_{DC/AC}$	0.0 ... 99.9 V	1.0 ... 1000 V	0.1 V	—	—	—	—	20M Ω	$\pm(8.6\% \text{ rdg.} + 9 \text{ d})$	$\pm(5\% \text{ rdg.} + 5 \text{ d})$	1200 V	cont.	
	100 ... 999 V		1 V										
	1.00 ... 1.2 kV		0.01 kV										
Frequency f_{\sim}	8.0 ... 99.9 Hz	10 ... 1000 Hz	0.1 Hz	—	—	—	—	20M Ω	$\pm(8.6\% \text{ rdg.} + 2 \text{ d})$	$\pm(2\% \text{ rdg.} + 1 \text{ d})$	1200 V	cont.	
	100 ... 999 Hz		1 Hz										

* Related to 10 A nominal current

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

Applicable Regulations and Standards

IEC 204-1 DIN EN 60204-1 VDE 0113 Part 1	Machine safety: Electrical equipment at machinery Part 1: General requirements
IEC 61010-1 DIN EN 61010-1 VDE 0411 Part 1	Safety requirements for electrical equipment for measurement, control and laboratory use – General requirements
DIN EN 60529 DIN VDE 0470-1	Protection provided by enclosures (IP code)
VDI/VDE 3540	Reliability of measuring, control and regulating devices – Climatic categories for devices and accessories
DIN 43 751 Part 1, 2	Digital measuring instruments
DIN EN 61 326-1	EMC – Generic standard for interference emission
DIN EN 61 326/A1	EMC – Generic standard for interference immunity

Regulations and Standards for Use of the Tester

IEC 204-1 DIN EN 60204-1 VDE 0113 Part 1	Machine safety: Electrical equipment at machinery – General requirements
DIN EN 60439-1 VDE 0660 Part 500	Low-voltage switchgear assemblies
DIN IEC 60-1, HD 588.1 VDE 0432 Part 1	High-voltage test methods
DIN EN 60335-1 DIN VDE 0700-1	Safety tests for household appliances Part 1: Safety of electrical devices for household use and similar purposes
DIN VDE 0701-1/5.93	Repair, modification and testing of electrical devices – General requirements
DIN VDE 0701-200/6.88	Mains powered electronic devices and accessories for household use and similar, general applications
DIN VDE 0701-240/4.86	Safety requirements for data processing systems and office machinery
DIN VDE 0701-260	Hand-held electric tools
DIN VDE 0472	Testing cables and insulated conductors
DIN VDE 0404-2/7.88	Devices for technical safety testing of electrical equipment – Devices for periodic testing

Reference Conditions

Line Voltage	230 V ± 1%
Line Frequency	50 Hz ± 0.1%
Waveshape	Sine (deviation between effective and rectified value < 1%)
Ambient Temperature	+ 23 °C ± 2 K
Relative Humidity	45% ... 55%
Load Impedance	Ohmic

Nominal Ranges of Use

Line Voltage	207 V ... 253 V
Line Frequency	45 Hz ... 65 Hz
Line Voltage Waveshape	Sine
Temperature Range	0 °C ... + 40 °C

Ambient Conditions

Storage Temperature	– 20 °C ... + 60 °C
Operating Temperature	– 5 °C ... + 40 °C
Accuracy	0 °C ... + 40 °C
Relative Humidity	Max. 75%, no condensation allowed
Elevation	to 2000 m

Power Supply

Line Voltage	207 V ... 253 V
Line Frequency	45 Hz ... 65 Hz
Power Consumption	204: approx. 180 VA <i>w/o accessories</i> 204HP: max. 700 VA 204HV: max. 100 VA
Max. Leakage Current	0.5 mA <i>basic device and 204HP or HV</i>
Current Consumption	Max. 6 A <i>basic device and 204HP or HV</i>

RS 232 Interface

Type	RS 232C, serial, per DIN 19241
Data Format	9600, 8, N, 1
Connector	9-pin subminiature socket connector

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

Electrical Safety

Safety Class	204: II 204HP/HV: I per IEC 61010-1/ EN 61010-1 and VDE 0411-1
Nominal Voltage	230 V
Test Voltage, 204	5.55 kV 50 Hz
Test Voltage, 204HP/HV	Mains /PE / key switch / external signal lamps to high voltage measuring terminals: 204HP: 5 kV AC 50 Hz 204HV: 8 kV AC 50 Hz
	Mains to PE: 1.5 kV AC
	Mains to external signal lamps: 2.3 kV AC (type test)
Overvoltage Category	II
Fouling Factor	2
EMC, Interference Emission	DIN EN 61326-1
EMC, Interference Immunity	DIN EN 61326/A1
Safety Shutdown	if instrument overheats
Fuses	204: Mains: T 1.6 / 250 Test probe: T16 / 1000 204HP/HV: Mains: F 3.15 / 250








Mechanical Design

Display	Multiple dot matrix display 128 x 128 pixels
Protection	IP 40 per DIN EN 60529 / VDE 0470 part 1
Dimensions	204: (WxDxH) 255 mm x 133 mm x 240 mm 204HP/HV: 254 mm x 130 mm x 285 mm overall height, mounted on caddy: 380 mm x 250 mm x 650 mm
Weight	204: approx. 5.1 kg 204HP/HV: approx. 8 kg

Standard Equipment

- 1 PROFITEST 204 test instrument with data interface (RS 232) and CENTRONICS port for external printer
- 1 test probe with integrated control panel for remote control of protective conductor and insulation measurement functions, with permanently attached measurement cable
- 1 test probe with integrated fuse and permanently attached measurement cable
- 1 cable lug
- 1 power cable with earthing contact plug
- 1 CD ROM with download program for report forms
- 1 maker's calibration certificate
- 1 RS232 bus cable for connecting the COM interface
- 1 operating instructions

Sample Displays, Menu-Driven Instrument Operation:

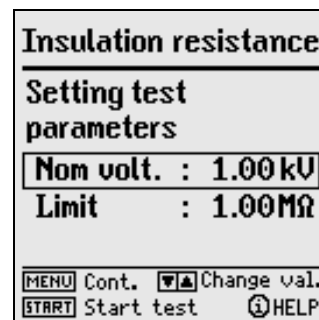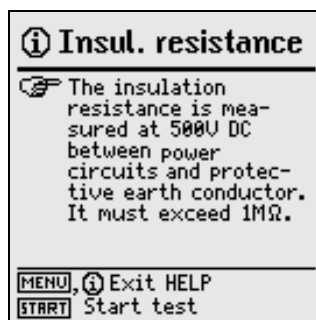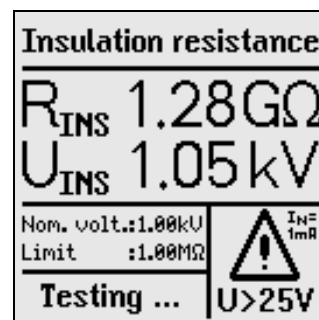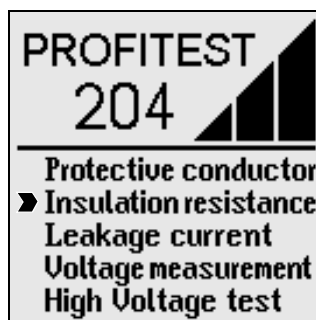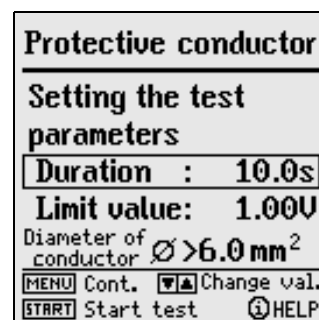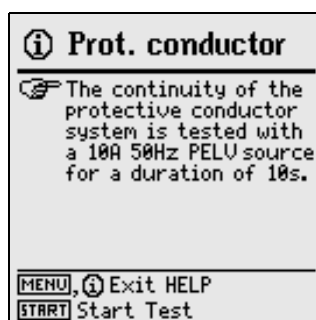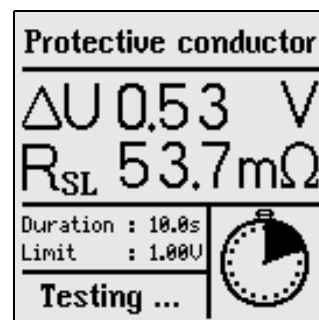

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

PROFITEST 204 Accessories

Expanded Features for PROFITEST 204HP-2.5kV and 204HV-5.4kV

- Test voltage selectable in 50 V steps
- Rise time (ramp) adjustable from 0.1 to 99 s
- Test duration adjustable from 1 to 120 s
- Floating test voltage outputs
- Electronically controlled test sequence
- Test sequence can be started with test pistol
- Breakdown voltage display
- Pulse-arc operation
- Phase angle display
- Measured values can be saved to memory
- Acoustic and optical error messages
- Key switch for protection against unauthorized start-up
- Connector terminals for external signal lamps

Expanded Features for PROFITEST 204HP-2.5kV

- Voltage test per EN 60204 / VDE 0113
- Test power: 500 VA (intermittent)
- Breaking current adjustable in 1 mA steps

Expanded Features for PROFITEST 204HV-5.4kV

- Test power: 50 VA
- Breaking current adjustable in 0.5 mA steps

Both of the high-voltage components, either of which can be mounted to the bottom of the basic instrument, allow for high-voltage testing. Voltage, current and phase angle are measured with permanently attached measurement cables. The bidirectional infrared interface at the base of the PROFITEST 204 is used for controlling the high-voltage component, as well as for uploading measured values to the basic instrument.




Technical Data, PROFITEST 204HP-2.5kV

	Nominal Range of Use	Resolution	Measuring Error	Intrinsic Error
Test Voltage U AC	250 V ... 2.5 kV	1 V 10 V	±(5% rdg. + 5 d)	±(2.5% rdg. + 5 d)
Meas. Quantity				
Current I AC	10.0 ... 200 mA	0.1 mA 1 mA	±(7% rdg. + 5 d)	±(5% rdg. + 5 d)

Technical Data, PROFITEST 204HV-5.4 kV

	Nominal Range of Use	Resolution	Measuring Error	Intrinsic Error
Test Voltage U AC	650 V ... 1.00 kV 1.00 kV ... 5.35 kV	1 V 10 V	+2 ... -7% rdg. +2 ... -5% rdg.	0 ... -5% rdg. 0 ... -3% rdg.
Meas. Quantity				
Current I AC	1.0 ... 10.0 mA	0.01 mA 0.1 mA	±(7% rdg. + 5 d)	±(5% rdg. + 5 d)

Sample Displays, Menu-Driven Instrument Operation:

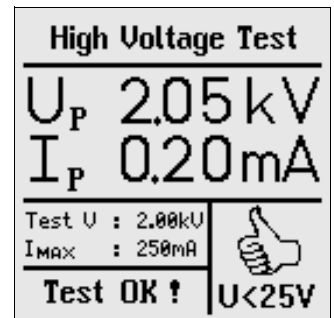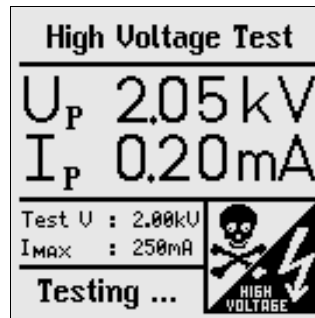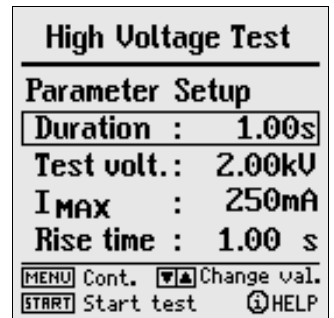

Extension PROFITEST 204HP...




Signal 204



Signal lamp set mounted to a magnetic base for high-voltage testing in accordance with DIN VDE 0104.

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

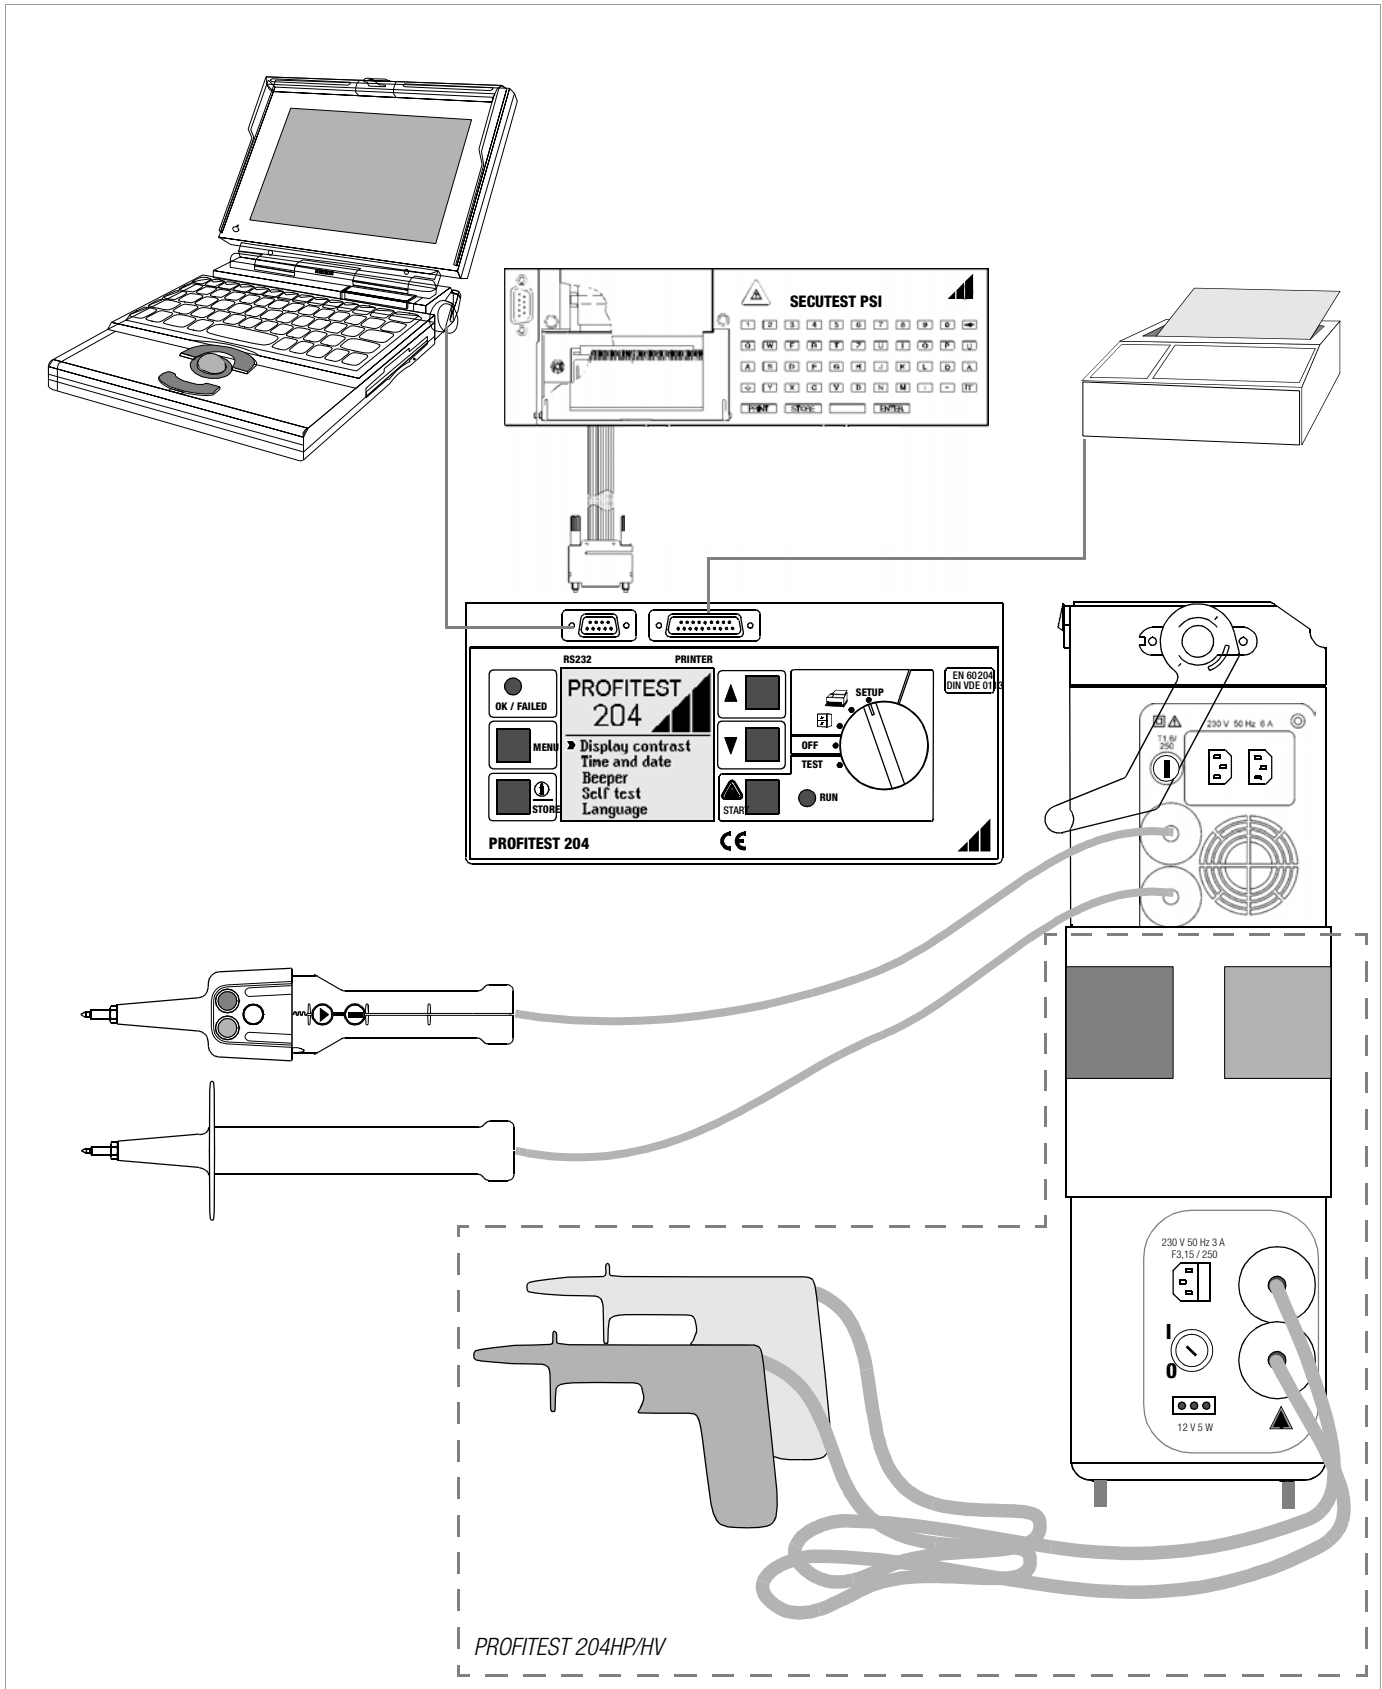

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

SECUTEST PSI

Values measured with the test instrument can be printed out with the help of this module. Beyond this, the alphanumeric keypad allows for the entry of descriptions for each individual system. Descriptions are automatically saved to memory along with the appropriate data record, and are printed out in the test report. The PSI module is screwed into the lid of the PROFITEST 204 for space-saving storage.



Caddy 204



PS3 Intelligent Modular Software for Test Instruments

Measurement data acquired with test instruments is transferred to PS3 and are then automatically assigned to activities such as testing, maintenance or inspection. Ready-to-sign test and work reports can thus be prepared with a minimum of effort.

The basic module and the device module are sufficient for standard requirements such as reading in measurement data and report printing.

Additional requirements such as following up on deadlines, test data history, data selection and list generation, right on up to complete object management (devices and buildings) with inventory management, errors indication, work orders and repairs are handled with the expansion module and with add-on modules.

An overview of all of the features included with this software is available in the PS3 brochure.


System requirements for PS3

- a Windows compatible PC with at least a Pentium CPU > 300 MHz
- MS-Windows 95 / 98 / NT 4.0
- 64 MB RAM Win 95/98; 128 MB RAM Win NT 4.0
- CD ROM drive
- a hard disc with approx. 150 MB free memory (without data)
- a floppy disc drive or e-mail connection for loading control and/or clearing files

REMOTE 204 (Windows software)

REMOTE 204 control software allows for automated test sequences with the help of a PC, including:

- Creation of control files for testing machines and systems
- Performance of testing in accordance with control files
- Reports generation
- Data export using a format which is compatible with all common spreadsheet programs

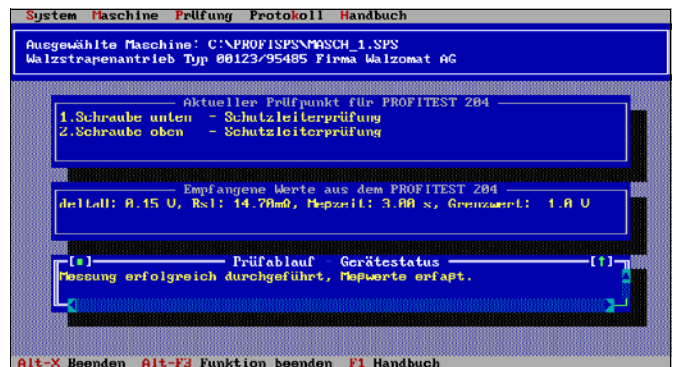

PROFITEST 204

Tester for DIN EN 60204 and VDE 0113

Order Information

Designation	Type	Article number
Device for tests in accordance with VDE 0113 / EN 60204 with RS232 interface and CENTRONICS port for external printer, 2 test probes firmly connected via measuring cables with a length of 4 m, 1 plug-on cable lug, power cable with earthing contact plug, floppy disc (D, GB, I, E, NL, DK, CZ) with download program for report forms, test report, operating instructions	PROFITEST 204	GTM 5027 000 R0001
Same test instrument as PROFITEST 204, however, with firmly connected measuring cable with a length of 12 m with START/MEMORY operation in the test plug	PROFITEST 204L	M505C
Sets		
Complete system for tests in accordance with DIN EN 60204-1/VDE 0113 part 1, consisting of: PROFITEST 204, PROFITEST 204HP, Signal 204, Leadex 204, Caddy 204, test report	MetraMachine 204/2.5	M504D
Complete system for tests in accordance with DIN EN 60204-1/VDE 0113 part 1, consisting of: PROFITEST 204, PROFITEST 204HP, Caddy 204, test report	MetraMachine 204-1/2.5	M504E
Complete system for tests in accordance with DIN EN 60439-1/VDE 0660 part 500, consisting of: PROFITEST 204, PROFITEST 204HV, Signal 204, Leadex 204 and Caddy 204, test report	MetraMachine 439/5.4	M504F
Extensions		
Special variant, High-voltage component to 2.5 kV	PROFITEST 204HP-2.5kV	M505A
Special variant, High-voltage component to 5.4 kV	PROFITEST 204HV-5.4kV	M505B
PSI-Modul including 2 rolls recording chart, 1 ink ribbon cartridge, batteries and operating instructions	SECUTEST PSI	GTM5016000R0001
Accessory equipment		
For securing sites against unauthorized presence during high-voltage testing	Claim 204-Set	Z504G
RS232 interface cable, 2 m	Z3241	GTZ 3241 000 R0001
Adapter for SL /ISO tests with PROFITEST 0100S-II and PROFITEST 204	Adapter 701	Z501F
Signal lamp set mounted on magnetic base for high-voltage testing in accordance with DIN VDE 0104	Signal 204	Z504D
Plug-on cable lug for secure attachment of the test probe to the terminals	Kabelschuh 204	Z504E

Designation	Type	Article number
12 m extension cable for use with the measurement cable and test probe with integrated measuring circuit fuse	Leadex 204	Z504C
Transport caddy for PROFITEST 204 and 204HP/HV, including rubber straps for securing test cables and protective cover	Caddy 204	Z504A
EMERGENCY STOP switch for PROFITEST 204HP/HV	STOP 204	Z504F
For securing sites against unauthorized presence during high-voltage testing	Claim 204	Z504G
Interface adapter for keyboards	PROFI-MFIL	Z504H
PS3 intelligent modular software for test instruments		
PROFITEST 204 device module	Z530D	Z530D
Basic module	Z531A	Z531A
Expansion module ¹⁾	Z531B	Z531B
Add-on modules ²⁾		
– LH Navigator + LH Viewer	Z531C	Z531C
– client compatibility	Z531D	Z531D
– inventory management STORE	Z531E	Z531E
– Repair management	Z531K	Z531K
– Network and multiple licenses	upon request	upon request
Control programming software in 3 languages for remote-control of PROFITEST/MACH 204 from the PC	REMOTE 204	Z532A
Pack of 10 rolls recording chart for PSI module (1 roll = approx. 6.7 m)	PS-10P	GTZ 3229 000 R0001
Pack of 10 ink ribbon cartridges for PSI module	Z3210	GTZ 3210 000 R0001
Universal carrying bag (for PROFITEST 204 and SECUTEST... without HV-module)	F2000 ^{D)}	Z700D

^{D)} Data sheet available

¹⁾ Prerequisite: device module and basic module

²⁾ Prerequisite: device module, basic module and add-on module

For further information on accessory equipment see our Catalog „Measuring Instruments and Testers“.

Printed in Germany • Subject to change without notice

GOSSEN-METRAWATT GMBH
 Thomas-Mann-Str. 16-20
 90471 Nürnberg, Germany
 Phone: +49 911 8602-0
 Fax: +49 911 8602-669
 e-mail: info@gmc-instruments.com
 http://www.gmc-instruments.com

GOSSEN
 METRAWATT
 CAMILLE BAUER