

Keysight Add Configurable Test Set Upgrade Kit

To Upgrade PNA N5224A or N5225A Option 400 to Option 401

Upgrade Kit Order Numbers: N5224AU-401 or N5225AU-401

Keysight Kit Number: N5225-60105

Notices

© Keysight Technologies, Inc.
2011-2015

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies, Inc. as governed by United States and international copyright laws.

Trademark Acknowledgments

Manual Part Number

N5225-90105

Edition

September 2015

Printed in USA/Malaysia

Published by:
Keysight Technologies
1400 Fountaingrove Parkway
Santa Rosa, CA 95403

Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED "AS IS," AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, KEYSIGHT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. KEYSIGHT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD KEYSIGHT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS

DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

U.S. Government Rights

The Software is "commercial computer software," as defined by Federal Acquisition Regulation ("FAR") 2.101. Pursuant to FAR 12.212 and 27.405-3 and Department of Defense FAR Supplement ("DFARS") 227.7202, the U.S. government acquires commercial computer software under the same terms by which the software is customarily provided to the public.

Accordingly, Keysight provides the Software to U.S. government customers under its standard commercial license, which is embodied in its End User License Agreement (EULA), a copy of which can be found at

<http://www.keysight.com/find/sweula>

The license set forth in the EULA represents the exclusive authority by which the U.S. government may use, modify, distribute, or disclose the Software. The EULA and the license set forth therein, does not require or permit, among other things, that Keysight: (1) Furnish technical information related to commercial computer software or commercial computer software documentation that is not customarily provided to the public; or (2) Relinquish to, or otherwise provide, the government rights in excess of these rights customarily provided to the public to use, modify, reproduce, release, perform, display, or disclose commercial computer software or commercial computer software documentation. No additional

government requirements beyond those set forth in the EULA shall apply, except to the extent that those terms, rights, or licenses are explicitly required from all providers of commercial computer software pursuant to the FAR and the DFARS and are set forth specifically in writing elsewhere in the EULA. Keysight shall be under no obligation to update, revise or otherwise modify the Software. With respect to any technical data as defined by FAR 2.101, pursuant to FAR 12.211 and 27.404.2 and DFARS 227.7102, the U.S. government acquires no greater than Limited Rights as defined in FAR 27.401 or DFAR 227.7103-5 (c), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

Keysight Add Configurable Test Set Upgrade Kit
Upgrade Kit Order Number: N5224AU-401 or N5225AU-401

Installation Note

Description of the Upgrade

This upgrade adds the following items to your N5224A Option 400 or N5225A Option 400 network analyzer:

- reference mixer switch
- front panel jumpers
- front panel jumpers cable guards
- front panel overlay replacement
- new cables

After installation of this upgrade, your analyzer will be an N5224A Option 401 or N5225A Option 401.

Getting Assistance from Keysight

By internet, phone, or fax, get assistance with all your test and measurement needs.

Contacting Keysight

Assistance with test and measurements needs and information on finding a local Keysight office are available on the Web at:

<http://www.keysight.com/find/assist>

If you do not have access to the Internet, please contact your Keysight field engineer.

NOTE

In any correspondence or telephone conversation, refer to the Keysight product by its model number and full serial number. With this information, the Keysight representative can determine whether your product is still within its warranty period.

Getting Prepared

CAUTION

The PNA contains extremely sensitive components that can be ruined if mishandled. Follow instructions carefully when making cable connections, especially wire harness connections.

The person performing the work accepts responsibility for the full cost of the repair or replacement of damaged components.

To successfully install this upgrade kit, you will need the following:

- A license key - refer to **“License Key Redemption”** below.
- A PDF copy or a paper copy of the PNA Service Guide - refer to **“Downloading the Online PNA Service Guide”** below.
- An ESD-safe work area - refer to **“Protecting Your Workspace from Electrostatic Discharge”** below.
- Correct tools - refer to **“Tools Required for the Installation” on page 7**.
- Enough time - refer to **“About Installing the Upgrade” on page 7**.
- Test equipment for the post-upgrade adjustments and full instrument calibration. To view the equipment list, click the Chapter 3 bookmark “Tests and Adjustments” in the PDF Service Guide¹.

License Key Redemption

NOTE

The enclosed Option Entitlement Certificate is a receipt, verifying that you have purchased a licensed option for the PNA of your choice. You must now use a Keysight Web page to request a license key for the instrument that will receive the option.

To enable the option product, you must request a license key from: <http://www.keysight.com/find/softwarelicense>. To complete the request, you will need to gather the following information:

- From the certificate
 - Order number
 - Certificate number
- From your instrument
 - Model number
 - Serial number
 - Host ID

1. See **“Downloading the Online PNA Service Guide” on page 6**.

Description of the Upgrade Getting Prepared

The instrument information is available on the network analyzer – on the analyzer's Help menu, click About Network Analyzer.

If you provide an email address, Keysight will promptly email your license key. Otherwise, you will receive your license key via postal mail.

Downloading the Online PNA Service Guide

To view the online Service Guide for your PNA model number, use the following steps:

1. Go to www.keysight.com.
2. In the Search box, enter the model number of the analyzer (Ex: N5242A) and click **Search**.
3. Click **Technical Support > Manuals**.
4. Click **Service Manual**.
5. Click the service guide title to download the PDF file.
6. When the PDF of the Service Guide is displayed, scroll through the Contents section bookmarks to locate the information needed.

Protecting Your Workspace from Electrostatic Discharge

For information, click on the Chapter 1 bookmark, “Electrostatic Discharge Protection” in the PDF Service Guide¹.

ESD Equipment Required for the Installation

Description	Keysight Part Number
ESD grounding wrist strap	9300-1367
5-ft grounding cord for wrist strap	9300-0980
2 x 4 ft conductive table mat and 15-ft grounding wire	9300-0797
ESD heel strap (for use with conductive floors)	9300-1308

Tools Required for the Installation

Description	Qty	Part Number
T-10 TORX driver - set to 9 in-lbs (1.02 N.m)	1	N/A
T-20 TORX driver - set to 21 in-lbs (2.38 N.m)	1	N/A
5/16-in (8 mm) nutsetter or open end torque wrench - set to 10 in-lbs (1.13 N.m)	1	N/A

CAUTION

Use a 5/16-in torque wrench set to 10 in-lbs on all cable connections.

About Installing the Upgrade

Products affected	N5224A and N5225A Option 400
Installation to be performed by	Keysight service center or personnel qualified by Keysight
Estimated installation time	2 hours
Estimated adjustment time	0.5 hours
Estimated full instrument calibration time	4.5 hours

1. See [“Downloading the Online PNA Service Guide”](#) on page 6.

Description of the Upgrade
Items Included in the Upgrade Kit

Items Included in the Upgrade Kit¹

Check the contents of your kit against the following list. If any part is missing or damaged, contact Keysight Technologies. Refer to **“Getting Assistance from Keysight” on page 4.**

Table 1 Contents of Upgrade Kit N5225-60105

Ref Desig.	Description	Qty	Part Number
--	Installation note (this document)	1	N5225-90105
A37	Reference mixer switch	1	5087-7759
--	Bracket (for A37 reference mixer switch)	1	N5245-00024
--	Machine screw, M3 x 8, pan head (2 to attach bracket to reference mixer switch; 2 to attach reference mixer switch assembly to deck)	5	0515-0372
--	Cable clamp	8	1400-1334
--	Cable guard	1	N5242-00030
--	Cable guard	2	N5242-00029
--	Front panel overlay	1	N5227-80005
W19	RF cable, A29 port 1 receiver coupler to front-panel Port 1 SOURCE OUT	1	N5245-20039
W20	RF cable, port 1 CPLR THRU to A33 port 1 coupler	1	N5245-20099
W21	RF cable, A29 port 1 receiver coupler to A37 reference mixer switch	1	N5245-20110
W22	RF cable, A33 port 1 coupler to front-panel Port 1 CPLR ARM	1	N5245-20014
W23	RF cable, A30 port 3 receiver coupler to front-panel Port 3 SOURCE OUT	1	N5245-20051
W24	RF cable, port 3 CPLR THRU to A34 port 3 coupler	1	N5245-20098
W25	RF cable, A30 port 3 receiver coupler to front-panel REF 3 SOURCE OUT	1	N5245-20016
W26	RF cable, A34 port 3 coupler to front-panel Port 3 CPLR ARM	1	N5245-20015
W27	RF cable, A31 port 4 receiver coupler to front-panel Port 4 SOURCE OUT	1	N5245-20052
W28	RF cable, port 4 CPLR THRU to A35 port 4 coupler	1	N5245-20096
W29	RF cable, A31 port 4 receiver coupler to front-panel REF 4 SOURCE OUT	1	N5245-20017
W30	RF cable, A35 port 4 coupler to front-panel port 4 CPLR ARM	1	N5245-20018
W31	RF cable, A32 port 2 receiver coupler to front-panel port 2 SOURCE OUT	1	N5245-20040
W32	RF cable, port 2 CPLR THRU to A36 port 2 coupler	1	N5245-20097

1. In addition to the upgrade kit, the shipment includes an Option Entitlement Certificate. Refer to **“License Key Redemption” on page 5** for important information about this certificate.

Description of the Upgrade
Items Included in the Upgrade Kit

Table 1 Contents of Upgrade Kit N5225-60105

Ref Desig.	Description	Qty	Part Number
W33	RF cable, A32 port 2 receiver coupler to front-panel REF 2 SOURCE OUT	1	N5245-20108
W34	RF cable, A36 port 2 coupler to front-panel port 2 CPLR ARM	1	N5245-20019
W36	RF cable, Front panel jumper	12	N5245-20155
W37	RF cable, port 1 RCVR A IN to A27 mixer brick (A)	1	N5245-20041
W38	RF cable, port 3 RCVR C IN to A28 mixer brick (C)	1	N5245-20037
W39	RF cable, port 4 RCVR D IN to A28 mixer brick (D)	1	N5245-20038
W40	RF cable, port 2 RCVR B IN to A27 mixer brick (B)	1	N5245-20042
W41	RF cable, A37 reference mixer switch to front-panel REF 1 RCVR R1 IN	1	N5245-20006
W42	RF cable, REF 1 SOURCE OUT to A37 reference mixer switch	1	N5245-20007
W43	RF cable, A37 reference mixer switch to A27 mixer brick (R1)	1	N5245-20009
W44	RF cable, REF 3 RCVR R3 IN to A28 mixer brick (R3)	1	N5245-20020
W45	RF cable, REF 4 RCVR R4 IN to 3 dB pad on A28 mixer brick (R4)	1	N5245-20021
W46	RF cable, REF 2 RCVR R2 IN to A27 mixer brick (R2)	1	N5245-20011
--	Ribbon cable, A23 test set motherboard J554 to A37 reference mixer switch	1	8121-0966

NOTE

Extra quantities of items such as protective plastic caps, screws, cable ties, and cable clamps may be included in this upgrade kit. It is normal for some of these items to remain unused after the upgrade is completed.

Installation Procedure for the Upgrade

The network analyzer must be in proper working condition prior to installing this option. Any necessary repairs must be made before proceeding with this installation.

WARNING

This installation requires the removal of the analyzer's protective outer covers. The analyzer must be powered down and disconnected from the mains supply before performing this procedure.

Overview of the Installation Procedure

- “Step 1. Obtain a Keyword and Verify the Information.”
- “Step 2. Remove the Outer Cover.”
- “Step 3. Remove the Front Panel Assembly.”
- “Step 4. Remove Some Existing Cables.”
- “Step 5. Remove a 3 dB Pad.”
- “Step 6. Assemble the A37 Reference Mixer Switch Assembly.”
- “Step 7. Install the A37 Reference Mixer Switch Assembly.”
- “Step 8. Install the New Cables.”
- “Step 9. Remove the Old Lower Front Panel Overlay.”
- “Step 10. Reinstall Front Panel Assembly.”
- “Step 11. Install the New Lower Front Panel Overlay.”
- “Step 12. Install Front Panel Jumpers.”
- “Step 13. Position the Cables and Wires to Prevent Pinching.”
- “Step 14. Reinstall the Outer Cover.”
- “Step 15. Enable Option 401.”
- “Step 16. Perform Post-Upgrade Adjustments and Calibration.”
- “Step 17. Prepare the PNA for the User.”

Step 1. Obtain a Keyword and Verify the Information

Follow the instructions on the Option Entitlement Certificate supplied to obtain a license key for installation of this upgrade. Refer to **“License Key Redemption” on page 5**.

Verify that the model number, serial number, and option number information on the license key match those of the instrument on which this upgrade will be installed.

If the model number, serial number, or option number do not match those on your license key, you will not be able to install the option. If this is the case, contact Keysight for assistance before beginning the installation of this upgrade. Refer to **“Contacting Keysight” on page 4**.

Once the license key has been received and the information verified, you can proceed with the installation at step 2.

Step 2. Remove the Outer Cover

For instructions, click the Chapter 7 bookmark “Removing the Covers” in the PDF Service Guide¹.

Step 3. Remove the Front Panel Assembly

For instructions, click the Chapter 7 bookmark “Removing and Replacing the Front Panel Assembly” in the PDF Service Guide¹.

Step 4. Remove Some Existing Cables

CAUTION

Be careful not to damage the center pins of the semirigid cables. Some flexing of the cables may be necessary but do not over-bend them.

1. Place the analyzer bottom-side up on a flat surface.
2. Remove the following cables. To see an image showing the location of these cables, click the Chapter 6 bookmark “Bottom RF Cables, Standard 4-Port Configuration, Option 400” in the PDF Service Guide².

These cables may be discarded - they will not be reinstalled.

- W107(N5224-20005) A29 port 1 receiver coupler to A27 mixer brick (R1)/3-dB pad
- W108(N5224-20024) A30 port 3 receiver coupler to A28 mixer brick (R3)
- W109(N5224-20027) A31 port 4 receiver coupler to A28 mixer brick (R4)/3-dB pad
- W110 (N5224-20028) A32 port 2 receiver coupler to A27 mixer brick (R2)
- W111(N5224-20013) A29 port 1 receiver coupler to A33 port 1 coupler
- W112(N5224-20015) A30 port 3 receiver coupler to A34 port 3 coupler
- W113(N5224-20016) A31 port 4 receiver coupler to A35 port 4 coupler
- W114(N5224-20014) A32 port 2 receiver coupler to A36 port 2 coupler
- W115(N5224-20022) A33 port 1 coupler to A27 mixer brick (A)

1. See **“Downloading the Online PNA Service Guide” on page 6**.
2. See **“Downloading the Online PNA Service Guide” on page 6**.

Description of the Upgrade
Installation Procedure for the Upgrade

- W116(N5224-20023) A34 port 3 coupler to A28 mixer brick (C)
- W117(N5224-20026) A35 port 4 coupler to A28 mixer brick (D)
- W118 (N5224-20025) A36 port 2 coupler to A27 mixer brick (B)

These cables must be saved - they will be reinstalled.

- W12 (N5245-20109) A29 port 1 receiver coupler to W11
- W14 (N5245-20043) A30 port 3 receiver coupler to W13
- W16 (N5245-20044) A31 port 4 receiver coupler to W15
- W18 (N5245-20111) A32 port 2 receiver coupler to W17

Step 5. Remove a 3 dB Pad

Remove and discard the 3 dB pad connected to A27 mixer brick port R1.

Step 6. Assemble the A37 Reference Mixer Switch Assembly


Mount the bracket (N5245-00024) to the reference mixer switch (5087-7759) using two screws (0515-0372). Use a T-10 TORX driver to tighten the screws. New parts are listed in **Table 1 on page 8**.

Step 7. Install the A37 Reference Mixer Switch Assembly

Refer to **Figure 1** for this step of the procedure. New parts are listed in **Table 1 on page 8**. Use a T-10 TORX driver to tighten all screws.

Figure 1

Reference Mixer Switch Assembly

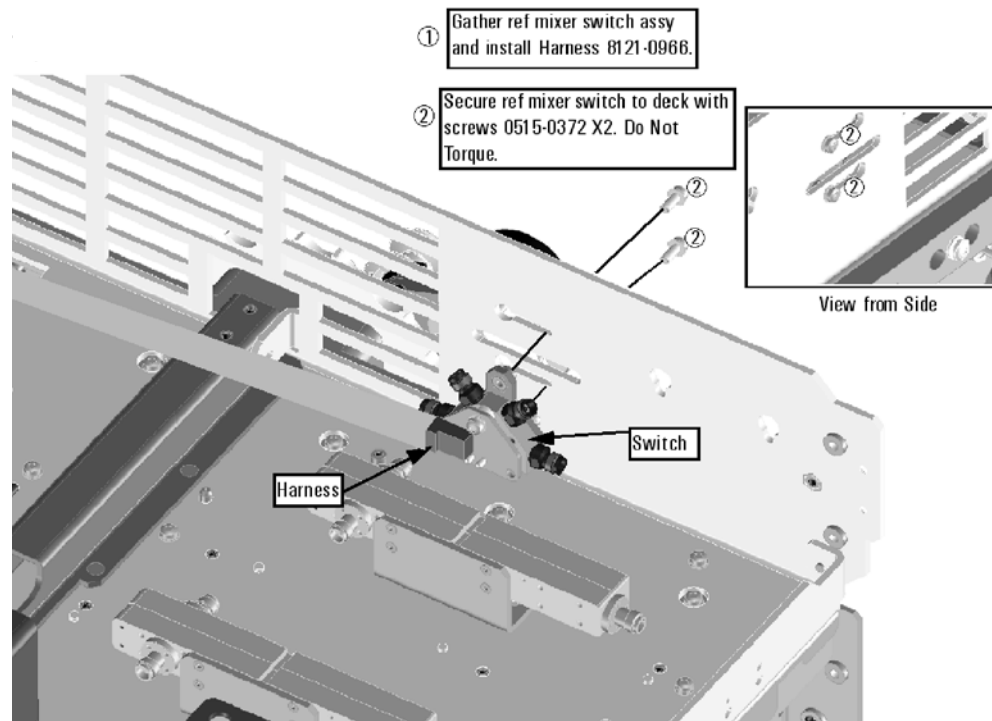

Step 8. Install the New Cables

CAUTION

Follow instructions carefully when making cable connections, especially wire harness connections. Incorrect connections can destroy components, resulting in additional customer costs.

Install the Semirigid Cables

To see an image showing the location of these cables, click the Chapter 6 bookmarks “Bottom RF Cables, 4-Port Configuration, Option 401” in the PDF Service Guide¹. New parts are listed in **Table 1 on page 8**.


Install the following new cables in the order listed.

- W40 (N5245-20042) Port 2 RCVR B IN to A27 mixer brick (B)

* As shown in **Figure 2 on page 14**, install one cable clamp (part number 1400-1334) to secure W40 (part number N5245-20042).

1. See **“Downloading the Online PNA Service Guide” on page 6**.

Figure 2 Location of Cable Clamp to Secure W40

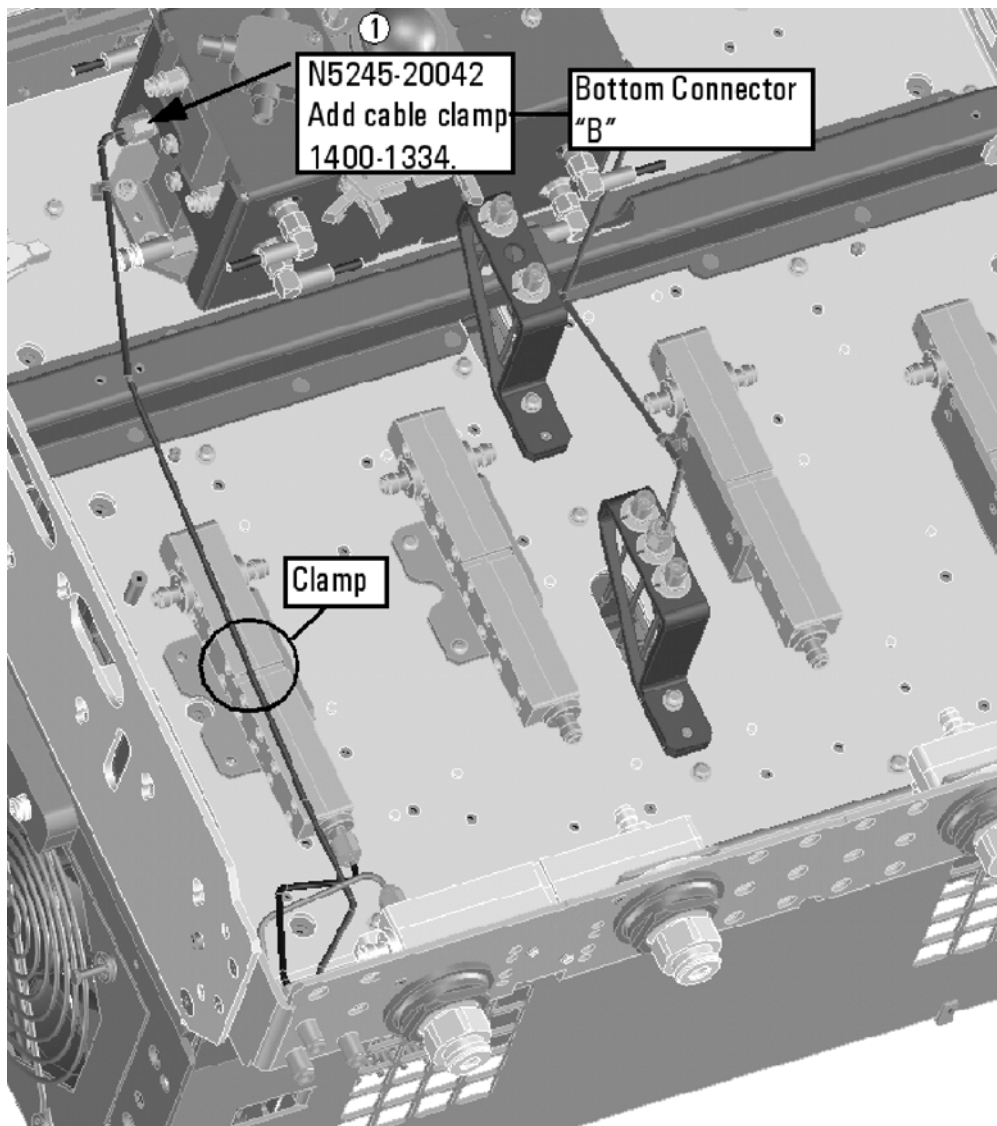


N5225_105_02

- W34 (N5245-20019) A36 port 2 coupler to front-panel port 2 CPLR ARM
- W31 (N5245-20040) A32 port 2 receiver coupler to front-panel port 2 SOURCE OUT
- W32 (N5245-20097) Port 2 CPLR THRU to A36 port 2 coupler
- W28 (N5245-20096) Port 4 CPLR THRU to A35 port 4 coupler
- W33 (N5245-20108) A32 port 2 receiver coupler to front-panel REF 2 SOURCE OUT

* As shown in [Figure 3 on page 15](#), install three cable clamps (part number 1400-1334) to secure W40 (part number N5245-20108).

Figure 3 Location of Cable Clamps to Secure W33

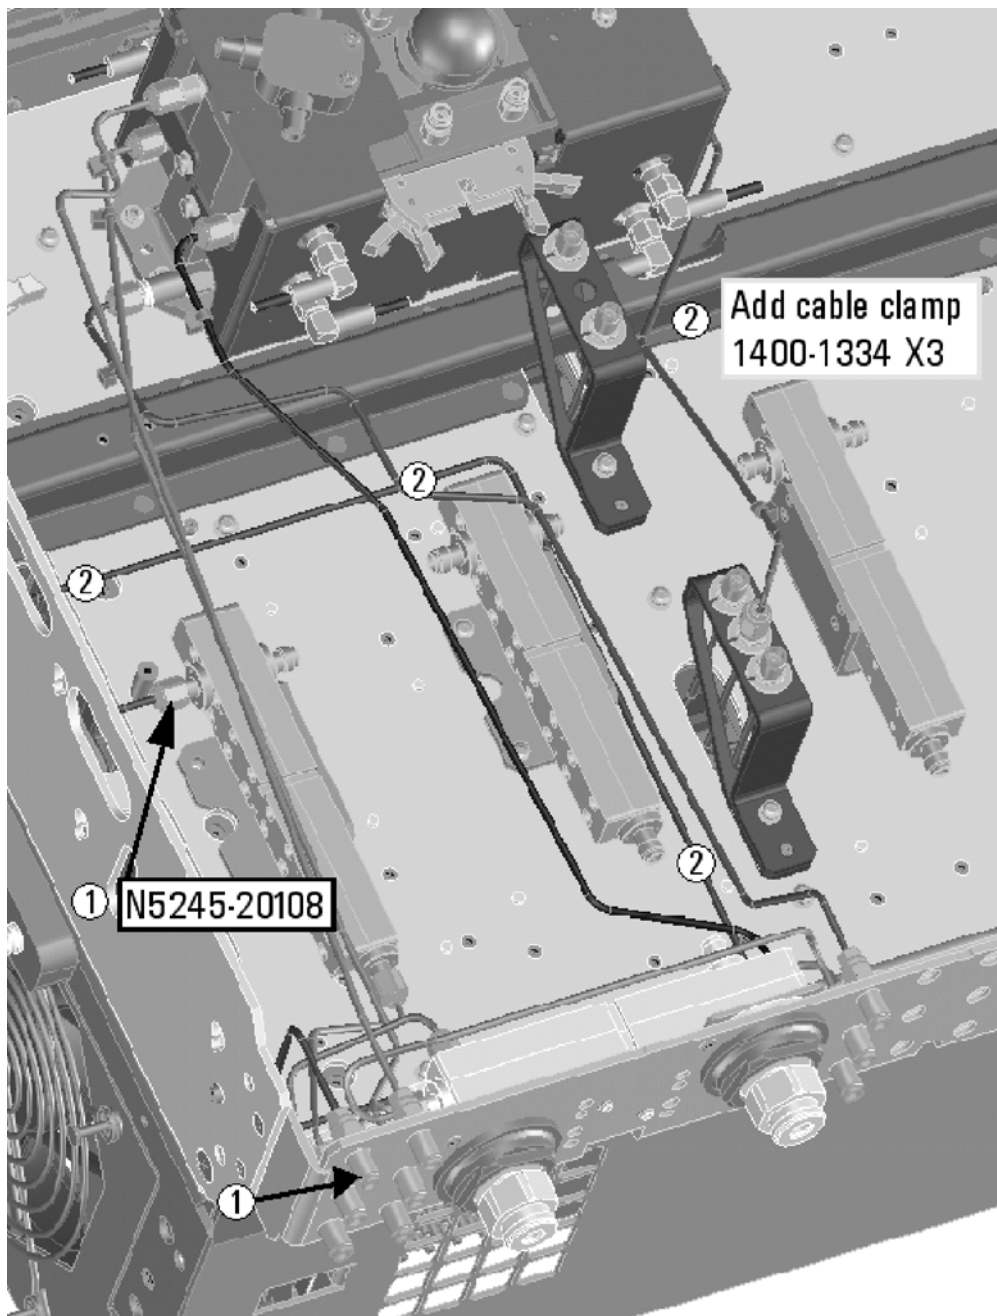

N5225_105_03

- W46(N5245-20011) REF 2 RCVR R2 IN to A27 mixer brick (R2)
- W39(N5245-20038) Port 4 RCVR D IN to A28 mixer brick (D)
- W45(N5245-20021) REF 4 RCVR R4 IN to 3 dB pad on A28 mixer brick (R4)
- W30(N5245-20018) A35 port 4 coupler to front-panel port 4 CPLR ARM
- W27 (N5245-20052) A31 port 4 receiver coupler to front-panel Port 4 SOURCE OUT

Description of the Upgrade
Installation Procedure for the Upgrade

- W29(N5245-20017) A31 port 4 receiver coupler to front-panel REF 4 SOURCE OUT
- W18(reuse) (N5245-20111) A32 port 2 receiver coupler to W17
- W38(N5245-20037) Port 3 RCVR C IN to A28 mixer brick (C)
- W44(N5245-20020) REF 3 RCVR R3 IN to A28 mixer brick (R3)
- W12(reuse) (N5245-20109) A29 port 1 receiver coupler to W11
- W20(N5245-20099) Port 1 CPLR THRU to A33 port 1 coupler
- W24 (N5245-20098) Port 3 CPLR THRU to A34 port 3 coupler
- W26 (N5245-20015) A34 port 3 coupler to front-panel Port 3 CPLR ARM
- W23 (N5245-20051) A30 port 3 receiver coupler to front-panel Port 3 SOURCE OUT
- W25(N5245-20016) A30 port 3 receiver coupler to front-panel REF 3 SOURCE OUT
- W37(N5245-20041) Port 1 RCVR A IN to A27 mixer brick (A)
- W22(N5245-20014) A33 port 1 coupler to front-panel Port 1 CPLR ARM
- W19(N5245-20039) A29 port 1 receiver coupler to front-panel Port 1 SOURCE OUT
- W42(N5245-20007) REF 1 SOURCE OUT to A37 reference mixer switch
- W41(N5245-20006) A37 reference mixer switch to front-panel REF 1 RCVR R1 IN
- W43(N5245-20009) A37 reference mixer switch to A27 mixer brick (R1)
- W21(N5245-20110) A29 port 1 receiver coupler to A37 reference mixer switch
- * **Figure 1 on page 13** shows two screws that attach the reference mixer switch to the test set deck. At this time, torque these two screws to 9 in-lbs.
- W14(reuse) (N5245-20043)A30 port 3 receiver coupler to W13
- W16(reuse) (N5245-20044)A31 port 4 receiver coupler to W15

Install the Ribbon Cable

To see an image showing the location of this cable, click the Chapter 6 bookmarks “Bottom Ribbon Cables and Wire Harnesses, 4-Port, Option 401” in the PDF Service Guide¹. New parts are listed in **Table 1 on page 8**.

If not already done, connect the reference mixer switch ribbon cable (8121-0966) as follows:

- A23 test set motherboard J554 to A37 reference mixer switch

1. See **“Downloading the Online PNA Service Guide” on page 6**.


Step 9. Remove the Old Lower Front Panel Overlay

Refer to **Figure 4** for this step of the procedure. Although this figure shows a 4-port PNA, the concept is the same for a 2-port PNA. New parts are listed in **Table 1 on page 8**.

1. From the back side of the front panel, use a blunt object in the cutouts in the lower front dress panel to push on the old overlay (item ①) and separate it from the front dress panel.
2. From the front side of the front panel, pull off the overlay completely and discard it.
3. Remove any adhesive remaining on the front panel.

Figure 4

Lower Front Panel Overlay Replacement

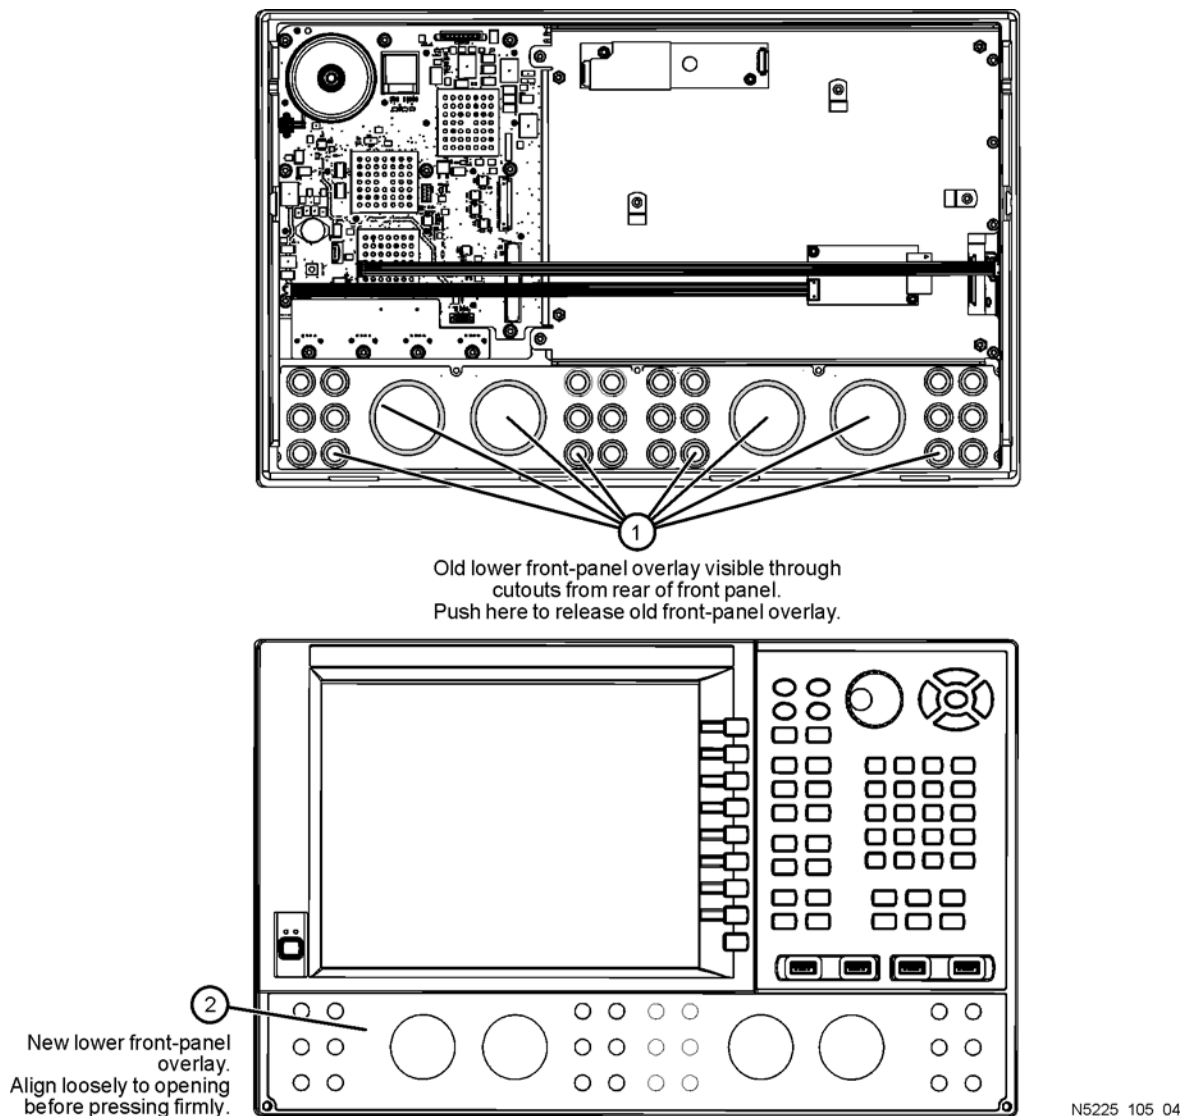

N5225_105_04

Step 10. Reinstall Front Panel Assembly

For instructions on reinstalling the front panel assembly, click the Chapter 7 bookmark “Removing and Replacing the Front Panel Assembly” in the PDF Service Guide¹.

Step 11. Install the New Lower Front Panel Overlay

Refer to **Figure 4 on page 17** for this step of the procedure. New parts are listed in **Table 1 on page 8**.

1. Remove the protective backing from the new front panel overlay, N5227-80005 (item ②).
2. Starting from either side, **loosely** place the overlay in the recess on the lower front panel, ensuring that it fits tightly against the edges of the recess.
3. Once the overlay is in place, press it firmly onto the frame to secure it.

Step 12. Install Front Panel Jumpers

As shown in **Figure 5**, install 12 front panel jumper cables (part number N5245-20155).

1. See **“Downloading the Online PNA Service Guide” on page 6**.

Figure 5 Front Panel Jumper Cables Installation



① **Install 6x jumper cables and torque to 10 in-lbs.**

N5225_105_05

Step 13. Position the Cables and Wires to Prevent Pinching

On the top side of the PNA, carefully position the grey flex cables so they can't be pinched between the covers and the rails.

On the bottom side of the PNA, carefully fold or push down the ribbon cables and wires so they can't be pinched between the hardware and the outer cover. Ribbon cables and wires must never be positioned on top of hardware.

Step 14. Reinstall the Outer Cover

For instructions, click the Chapter 7 bookmark "Removing the Covers" in the PDF Service Guide¹.

Step 15. Enable Option 401

Procedure Requirements

- The analyzer must be powered up and operating to perform this procedure.
- The Network Analyzer program must be running.
- A keyboard must be connected to the network analyzer.

Option Enable Procedure

1. To start the option enable utility, press UTILITY **System**, then **Service**, then **Option Enable**. An option enable dialog box will appear.
2. Click the arrow in the Select Desired Option box. A list of available options will appear.
3. In the Select Desired Option list, click 401 - Configurable Test Set.
4. Using the keyboard, enter the license key in the box provided. The license key is printed on the license message you received from Keysight. Enter this key exactly as it is printed on the message.
5. Click Enable.
6. Click Yes in answer to the displayed question in the Restart Analyzer? box.
7. When the installation is complete, click Exit.

Option Verification Procedure

Once the analyzer has restarted and the Network Analyzer program is again running:

1. On the analyzer's Help menu, click About Network Analyzer.
2. Verify that "401" is listed after "Options:" in the display. Click OK.

NOTE

If Option 401 has not been enabled, perform the **"Option Enable Procedure"** again. If the option is still not enabled, contact Keysight Technologies. Refer to **"Getting Assistance from Keysight" on page 4**.

Step 16. Perform Post-Upgrade Adjustments and Calibration

Adjustments

The following adjustments must be made due to the hardware changes of the analyzer.

- source adjustment
- receiver adjustment

These adjustments are described in the PNA Service Guide and in the PNA on-line HELP. A list of equipment required to perform these adjustments is also found in the service guide.

To view this service guide information, click the Chapter 3 bookmark "Tests and Adjustments" in the PDF Service Guide¹.

1. See **"Downloading the Online PNA Service Guide" on page 6**.

Description of the Upgrade
Installation Procedure for the Upgrade

After the specified adjustments have been performed, the analyzer should operate and phase lock over its entire frequency range.

Operator's Check

Perform the Operator's Check to check the basic functionality of the analyzer. For instructions, click the Chapter 3 bookmark "Tests and Adjustments" in the PDF Service Guide¹.

If you experience difficulty with the basic functioning of the analyzer, contact Keysight. Refer to **"Contacting Keysight" on page 4**.

Calibration

Although the analyzer functions, its performance relative to its specifications has not been verified. It is recommended that a full instrument calibration be performed using the analyzer's internal performance test software. To view information on the performance test software, click the Chapter 3 bookmark "Tests and Adjustments" in the PDF Service Guide¹.

Step 17. Prepare the PNA for the User

1. If necessary, reinstall front jumper cables.
2. Install the cable guards, pushing them over the front jumper cables until the cushioning material touches the front panel of the PNA.
3. Install the dust caps on the test ports.
4. Clean the analyzer, as needed, using a damp cloth.

This information is subject to change without notice.

© Keysight Technologies 2011 - 2015

September 2015



N5225-90105
www.keysight.com