Keysight U1731C/U1732C/U1733C Handheld LCR Meter

Quick Start Guide



NOTICE: This document contains references to Agilent Technologies. Agilent's former Test and Measurement business has become Keysight Technologies. For more information, go to **www.keysight.com.**



Keysight U1731C/U1732C/U1733C Handheld LCR Meter

Quick Start Guide



Verify that you received the following items in the shipment of your LCR meter:

- One pair of alligator clip test leads
- ✓ One 9 V alkaline battery
- Printed copy of the U1731C/U1732C/U1733C Quick Start Guide
- Printed copy of the Certificate of Calibration

If any item is missing or damaged, keep the shipping materials and contact the nearest Keysight Sales Office.

NOTE

The descriptions and instructions in this guide apply to the U1731C. U1732C. and U1733C handheld LCR meters.

The model U1733C appears in all illustrations.

All related documents and software are available for download at www.keysight.com/find/hhTechLib.



U1731C/U1732C/U1733C Handheld LCR Meter

Install the Batteries

Install the Batteries

Your LCR meter is powered by a single 9 V alkaline battery (included with the shipment).

- Turn the LCR meter OFF and remove the test leads from the terminals.
- 2 Lift the tilt stand and loosen the screw with a suitable Phillips screwdriver.
- 3 Remove the battery cover and observe the polarity markings.
- 4 Insert the battery and replace the battery cover and screw.



Turn On the LCR Meter

To power ON your LCR meter, press the power-on button once.





To avoid damage to the device, do not exceed the input limit. Do not apply voltage to the input terminals. Discharge the capacitor before testing.



Your LCR meter is capable of remote data logging. To use this feature, you will need an IR-USB cable (U5481A, purchased separately) and the Keysight GUI Data Logger Software (downloadable from www.keysight.com/find/hhTechLib).

The LCR Meter at a Glance



The external AC to DC power adapter input jack requires an input voltage of +12 VDC.

U1731C/U1732C/U1733C Handheld LCR Meter

Understanding the Keypad

Understanding the Keypad

Legend	Key response when pressed for:	
	Less than 1 second	More than 1 second
	Turns the LCR meter on or off	-
Ai A ESR	Starts or stops the auto identification mode	Enables or disables the ESR (equivalent series resistance) mode ^[1]
Hold Rec Save	Holds or releases the present reading on the display	Starts or stops the static recording mode
DQ⊖ Limit ◀	Switches between dissipation factor (D), quality factor (Q), and phase angle (θ) measurement	Enables or disables the limit comparison mode
Freq.	Selects a test frequency	Enables or disables the DCR (direct current resistance) mode ^[2]
Range > Auto	Disables autoranging and sets a manual range	Enables autoranging
ZLCR P⇔S	Switches between impedance (Z), inductance (L), capacitance (C), and resistance (R) measurement	Toggles between parallel and series circuit mode
Tol%	Enables the tolerance mode	Turns the backlight display on or off ^[3] or disables the tolerance mode (if tolerance is enabled)
A Null Cal	Sets the null/relative mode	Enters the open/short calibra- tion mode for selected range and test frequency

^[1] Autoranging only. ESR mode exits to capacitance (C) measurement by default.

 $^{^{[2]}}$ Applicable for U1733C model only. DCR mode exits to inductance (L) measurement by default.

^[3] Applicable for U1732C and U1733C models only.

Performing LCR Measurements

Auto Identification (Ai)


Press the $\begin{subarray}{l} A^* button to automatically identify and select an appropriate primary measurement function (L, C, or R), secondary measurement function (D, Q, or <math>\theta$), and measurement mode (parallel or series) for the device-under-test.

NOTE

The LCR meter powers up in the Ai mode by default. shown on the left of the display screen when the Ai mode is enabled.

- It flashes when the LCR meter is identifying a measurement function and mode
- Press A again while A is shown to exit the Ai mode.

LCR measurement steps

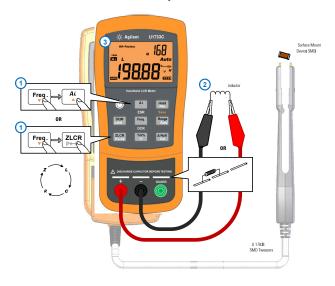

U1731C/U1732C/U1733C Handheld LCR Meter

Performing LCR Measurements

Secondary (D/Q/ θ) measurements





Inductance (L) measurements





Capacitance (C) measurements





Resistance (R) measurements





Contacting Keysight

To obtain service, warranty or technical assistance, contact us at the following phone numbers:

· United States Call Center: 800-829-4444

Canada Call Center: 877-894-4414
China Call Center: 800-810-0189
Europe Call Center: 31-20-547-2111
Japan Call Center: (81) 426-56-7832

For other countries, contact your country's Keysight support organization. A list of contact information for other countries is available on the Keysight Web site: www.keysight.com/find/assist

Safety Notices

CAUTION

A CAUTION notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING

A WARNING notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

Safety Information

This meter is safety-certified in compliance with the following safety and EMC requirements:

- IEC61010-1:2001/EN61010-1:2001 (Second Edition)
- IEC 61326-1:2005/ EN 61326-1:2006
- Canada: ICES/NMB-001:Issue 4, June 2006
- Australia/New Zealand: AS/NZS CISPR11:2004

Safety Symbols

≐	Earth (ground) terminal
	Equipment protected throughout by double insulation or reinforced insulation
A	Caution, risk of electric shock
Ŵ	Caution, risk of danger (refer to the instrument manual for specific Warning or Caution information)

This information is subject to change without notice. © Keysight Technologies 2014 Edition 4, August 2014





