


Making High-Accuracy Temperature Measurements With the 34970A Data Acquisition Switch Unit

Application Note 1425

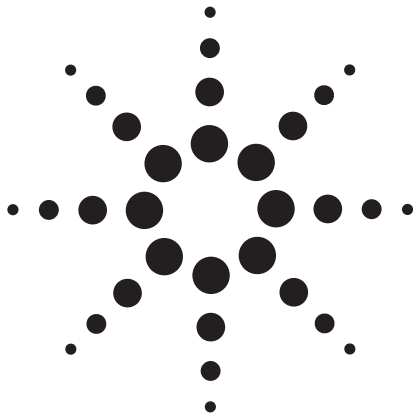

Introduction

If you want to make more accurate measurements with your Agilent 34970A data acquisition switch unit and the Agilent 34901A 20-channel multiplexer module, you can use an external isothermal terminal panel, or “patch panel,” such as the E1586A rack-mount terminal panel available from VXI Technology (www.vxitech.com). The E1586A is an aluminum isothermal terminal block that allows you to make temperature measurements with less than $\pm 0.53\text{ }^{\circ}\text{C}$ error. The accuracy of relative measurements is better than $\pm 0.35\text{ }^{\circ}\text{C}$ across 39 channels.

This application note explains how to wire the E1586A remote isothermal panel and use it to make high-accuracy temperature measurements with a 34970A data acquisition switch unit and 34901A 20-channel multiplexer module.

Wiring the E1586A remote isothermal panel

The E1586A remote isothermal panel is designed for up to 32 channels with three wires per channel (HI, LO, GND) and comes from the factory with the front panel markings for three-wire channels.

Front panels manufactured after Jan. 1, 2003 also have a silk-screened diagram on the rear of the panel for up to 48 two-wire channels. To use these two-wire markings with the 34970A, remove the two screws, turn the panel over (left to right) and replace the screws. On this panel, the channels are divided into two sections with 24 channels each. One E1586A panel can be used with a 34901A module to measure 19 Channels. The first channel in the 34901A module is used to measure the reference temperature, leaving 19 channels for thermocouple measurements. A second 34901A module can be added to measure up to 39 channels with a single E1586A panel.

When used with the 34970A and 34901A module you will want to use the two-wire markings. The right side of the panel has the channels configured the same way; you can use it with a second 34901A module.

To wire the panel to one 34901A MUX module, you need a SCSI cable. One SCSI cable can accommodate one 34901A module (20 channels). The first channel of the first 34901A module is required for the thermistor reference on the

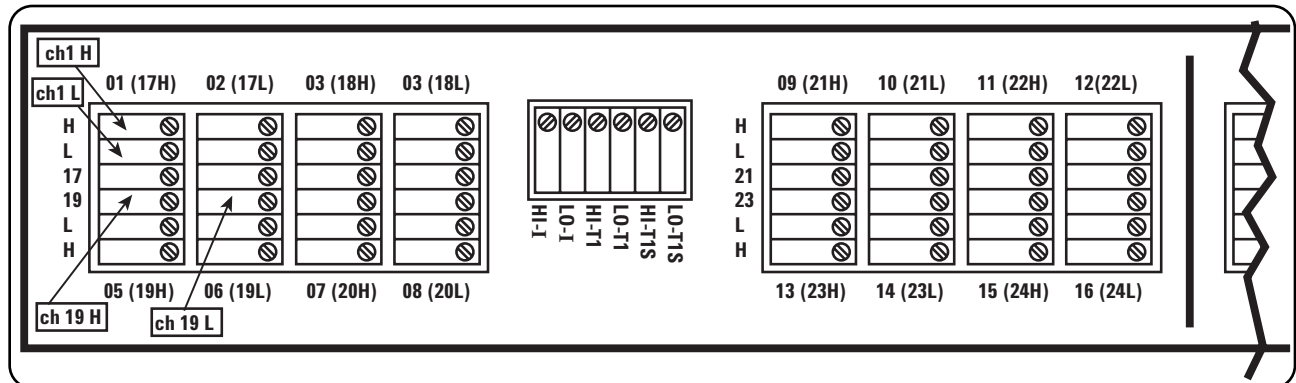


Figure 1: Left side of the E1586A terminal panel, shown with two-wire markings

34901A channel	Twisted pair First color is solid color	Painted left, J19	Painted right, J20	Aluminium left, J19	Aluminium right, J20
Ch01 H Ch01 L	Brown/white White/brown	0 HI 0 LO	16 HI 16 LO	Ch 01 H Ch 01 L	Ch 01 H Ch 01 L
Ch02 H Ch02 L	Brown/orange Orange/brown	1 HI 1 LO	17 HI 17 LO	Ch 02 H Ch 02 L	Ch 02 H Ch 02 L
Ch03 H Ch03 L	Brown/yellow Yellow/brown	2 HI 2 LO	18 HI 18 LO	Ch 03 H Ch 03 L	Ch 03 H Ch 03 L
Ch04 H Ch04 L	Brown/blue Blue/brown	3 HI 3 LO	19 HI 19 LO	Ch 04 H Ch 04 L	Ch 04 H Ch 04 L
Ch05 H Ch05 L	Brown/violet Violet/brown	4 HI 4 LO	20 HI 20 LO	Ch 05 H Ch 05 L	Ch 05 H Ch 05 L
Ch06 H Ch06 L	Tan/brown Brown/tan	5 HI 5 LO	21 HI 21 LO	Ch 06 H Ch 06 L	Ch 06 H Ch 06 L
Ch07 H Ch07 L	Tan/white White/tan	6 HI 6 LO	22 HI 22 LO	Ch 07 H Ch 07 L	Ch 07 H Ch 07 L
Ch08 H Ch08 L	Tan/orange Orange/tan	7 HI 7 LO	23 HI 23 LO	Ch 08 H Ch 08 L	Ch:08 H Ch 08 L
Ch09 H Ch09 L	Tan/yellow Yellow/tan	8 HI 8 LO	24 HI 24 LO	Ch 09 H Ch 09 L	Ch 09 H Ch 09 L
Ch 10 H Ch 10 L	Tan/blue Blue/tan	9 HI 9 LO	25 HI 25 LO~	Ch 10 H Ch 10 L	Ch 10 H Ch 10 L
Ch 11 H Ch 11 L	Tan/violet Violet/tan	10 HI 10 LO	26 HI 26 LO	Ch 11 H Ch 11 L	Ch 11 H Ch 11 L
Ch 12 H Ch 12 L	White/pink Pink/white	11 HI 11 LO	27 HI 27 LO	Ch 12 H Ch 12 L	Ch 12 H Ch 12 L
Ch 13 H Ch 13 L	White/orange Orange/white	12 HI 12 LO	28 HI 28 LO	Ch 13 H Ch 13 L	Ch 13 H Ch 13 L
Ch 14 H Ch 14 L	White/green Green/white	13 HI 13 LO	29 HI 29 LO	Ch 14 H Ch 14 L	Ch 14 H Ch 14 L
Ch 15 H Ch 15 L	White/blue Blue/white	14 HI 14 LO	30 HI 30 LO	Ch 15 H Ch 15 L	Ch 15 H Ch 15 L
Ch 16 H Ch 16 L	White/gray Grey/white	15 HI 15 LO	31 HI 31 LO	Ch 16 H Ch 16 L	Ch 16 H Ch 16 L
Ch 17 H Ch 17 L	Brown/pink Pink/brown	0 G 1 G	16 G 17 G	Ch 17 H Ch 17 L	Ch 17 H Ch 17 L
Ch 18 H Ch 18 L	Brown/green Green/brown	2 G 3 G	18 G 19 G	Ch 18 H Ch 18 L	Ch 18 H Ch 18 L
Ch 19 H Ch 19 L	Brown/gray Gray/brown	4 G 5 G	20 G 21 G	Ch 19 H Ch 19 L	Ch 19 H Ch 19 L
Ch 20 H Ch 20 L	Tan/pink Pink/tan	6 G 7 G	22G 23 G	Ch 20 H Ch 20 L	Ch 20 H Ch 20 L
Not used	Tan/green Green/tan	8 G 9 G	24 G 25 G	Ch 21 H Ch 21 L	Ch 21 H Ch 21 L
Not used	Tan/gray Gray/tan	10 G 11 G	26 G 27 G	Ch 22 H Ch 22 L	Ch 22 H Ch 22 L
Ch01 H Ch01 L	White/yellow Yellow/white	12 G 13 G	28 G 29 G	Ch 23 H Ch 23 L	Ch 23 H Ch 23 L
Not used	White/violet Violet/white	14 G 15 G	30 G; 31 G	Ch 24 H Ch 24 L	Ch 24 H Ch 24 L
Earth Earth	Orange/pink Pink/orange	I-Hi I-Lo	Trig Gnd	I-Hi I-Lo	Trig Gnd

Table 1: Wiring table

Caution: Your cable may have different color codes for each wire. This is a Computer Cable Makers PN SCS2-1000-003 wiring table.

E1586A and will therefore provide 19 channels of thermocouple measurements. A second 34901A module and a second cable will provide another 20 channels for a total of 39 thermocouple channels and one channel for the thermistor reference.

The SCSI cable must have 25 color-coded twisted pairs, a HD-50 male metal connector on one end and no connector on the other end. An 80 cm (2.5 ft) SCSI-2 to SCSI-1 cable is available for about US\$20.00 from Computer Cable Makers (www.cablemakers.com, PN SCS2-1000-003) and from Cables to Go (www.cablestogo.com).

Wiring is straightforward. Insert the cable into J19 on the left rear of the E1586A terminal panel and cut off the connector on the other end of the cable. Strip the outer insulation back about 20 cm (8 in). Strip the outer and inner shield back 19 cm (7.5 in). Fold the outer shield back on the insulation and cover it with heat shrink. Insert the cable in the 34901A module and fasten it with a tie wrap.

Connect an ohmmeter set to continuity and make contact with the H side of channel 1. Find the corresponding twisted pair (brown/org, org/brown), strip both wires, and check to make sure it is the correct wire pair. Now cut the pair to the proper length and insert in the channel 1H and 1L of the module. Repeat for channel 2-20. Similarly wire another cable and module to the right side of the panel (J20) for channels 21 to 40. Wire the twisted pair indicated in Table 1 to Earth in both of the 34901A modules.

On the first 34901A module, reduce the resistance of channel 1 to below 0.5 ohm by connecting the twisted pair in the cable for channel 23 to channel 1 of the 34901A terminal block. This will parallel two twisted wire pairs for channel one. See wiring table.

To connect the reference thermistor on the E1586A, connect channel 01H and 23H to HI-T2S, and channel 01L and 23L to LO-T2S.

To connect the shield and the ground on the E1586A, connect together HI-I, LO-I, GND, and TRIG. The wiring from the 34901A module to the E1586A is now complete. See the wiring table for detailed connections.

Wire the thermocouple wires to the channels corresponding to the channels in the 34901A modules. See the wiring table for panel labeling.

Making accurate temperature measurements

You can mount the E1586A terminal panel in a standard-size instrument rack or place it on your bench. To minimize any variation between channels, keep the terminal panel away from heat sources and drafts. Do not place the terminal panel directly next to instruments, or directly on top of a powered instrument. To isolate the panel from any heat source beneath the panel, place a section of foam or Styrofoam under the full length of the terminal panel. To protect the terminal panel from drafts, cover or wrap it in a towel or cloth or surround it with Styrofoam.

When you mount the terminal panel in a rack, mount it away from heat sources. The bottom of the rack is usually best. Take particular care to minimize the temperature difference across the horizontal width of the terminal panel, since it is most susceptible to horizontal temperature gradients across its longest dimensions. Avoid mounting the terminal panel directly above or below instruments that have hot air exits on their sides.

Channels closest to the center near the reference thermistor will have the best accuracy. When relative measurements are important, put those channels physically close together on the terminal panel. Channels closest together will have the best agreement among each other.

Table 2 shows the measurement uncertainty for the individual error contributions when you use a J-type thermocouple. The errors for other thermocouples

Source of error	Absolute accuracy J type	Relative accuracy J type
Isothermal termination, E1586A	$\pm 0.2^{\circ}\text{C}$ ($\pm 10\mu\text{V}$)	0.2°C difference across 40 channels
Thermocouple conversion	$\pm 0.05^{\circ}\text{C}$	$\pm 0.05^{\circ}\text{C}$
Ref. Thermistor Measurement	$\pm 0.08^{\circ}\text{C}$	N/A
Ref. Thermistor accuracy	$\pm 0.1^{\circ}\text{C}$	N/A
Ref. Thermistor lead resistance	- 0.003°C (< 0.5 ohms)	N/A
Voltmeter accuracy	$\pm 0.08^{\circ}\text{C}$ ($\pm 4\mu\text{V}$ @ 0.0mV), 25°C	$\pm 0.1^{\circ}\text{C}$ ($\pm 5\mu\text{V}$ @ 26 mV), 500°C
Total	$\pm 0.53^{\circ}\text{C}$ not including sensor	$\pm 0.35^{\circ}\text{C}$ not including sensor

Table 2: Measurement uncertainty

and temperature ranges will be different depending on the error of the voltmeter, the temperature measured, thermocouple type and voltage level of the thermocouple. The error due to the thermocouple is not included in the calculation.

Summary

If you use the E1586A patch panel with the 34970A and 34901A MUX module, your temperature measurement accuracy will be about twice as good as it is without the patch panel.

Glossary

J-type thermocouple – iron-constantan thermocouple with a temperature range of -210 to 1200°C

Thermocouple – a temperature sensor consisting of two dissimilar metals joined together. When a temperature gradient exists (one end is a different temperature from the other), a voltage is generated. Different types of thermocouples are constructed from different metals, with differing temperature ranges and accuracies.

Thermistor – a ceramic temperature sensor that exhibits a change in resistance as a function of temperature. With most thermistors, resistance decreases as the temperature increases.

Related Agilent Literature

Product overview – 34970A Data Acquisition/Switch Unit, pub. no.5965-5290EN

Application Note 290 – Practical Temperature Measurements, pub. no. 5965-7822E

Agilent Email Updates

www.agilent.com/find/emailupdates

Get the latest information on the products and applications you select.

Agilent T&M Software and Connectivity

Agilent's Test and Measurement software and connectivity products, solutions and developer network allows you to take time out of connecting your instruments to your computer with tools based on PC standards, so you can focus on your tasks, not on your connections. Visit www.agilent.com/find/connectivity for more information.

By internet, phone, or fax, get assistance with all your test and measurement needs

Online assistance: www.agilent.com/find/assist

Phone or Fax

United States:
(tel) 800 452 4844

Canada:
(tel) 877 894 4414
(fax) 905 282 6495

China:
(tel) 800 810 0189
(fax) 800 820 2816

Europe:
(tel) (31 20) 547 2323
(fax) (31 20) 547 2390

Japan:
(tel) (81) 426 56 7832
(fax) (81) 426 56 7840

Korea:
(tel) (82 2) 2004 5004
(fax) (82 2) 2004 5115

Latin America:
(tel) (305) 269 7500
(fax) (305) 269 7599

Taiwan:
(tel) 0800 047 866
(fax) 0800 286 331

Other Asia Pacific Countries:
(tel) (65) 6375 8100
(fax) (65) 6836 0252
(e-mail) tm_asia@agilent.com

Product specifications and descriptions in this document subject to change without notice.

© Agilent Technologies, Inc. 2003
Printed in the USA April 28, 2003
5988-8152EN

