

# **Agilent InfiniiVision 2000/3000 X-Series Oscilloscopes**

## **Service Guide**



**Agilent Technologies**

# Notices

© Agilent Technologies, Inc. 2008-2012

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Agilent Technologies, Inc. as governed by United States and international copyright laws.

## Manual Part Number

75019-97039, February 2012

Print History:  
75019-97012, January 2011  
75019-97015, July 2011  
75019-97039, October 2011

Available in electronic format only

Agilent Technologies, Inc.  
1900 Garden of the Gods Road  
Colorado Springs, CO 80907 USA

**A newer version of this manual may be available at**

[www.agilent.com/find/3000X-Series-manual](http://www.agilent.com/find/3000X-Series-manual)

Microsoft<sup>®</sup> is a U.S. registered trademark of Microsoft Corporation.

## Warranty

**The material contained in this document is provided “as is,” and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.**

## Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

## Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as “Commercial computer software” as defined in DFAR 252.227-7014 (June 1995), or as a “commercial item” as defined in FAR 2.101(a) or as “Restricted computer software” as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies’ standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as

defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

## Safety Notices

### CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

### WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

# In This Service Guide

This book provides the service information for the Agilent 2000/3000 X-Series oscilloscopes. This manual is divided into these chapters:

## **1 Characteristics and Specifications**

This chapter contains a partial list of characteristics and specifications for the Agilent InfiniiVision 2000/3000 X-Series oscilloscopes.

## **2 Testing Performance**

This chapter explains how to verify correct oscilloscope operation and perform tests to ensure that the oscilloscope meets the performance specifications.

## **3 Calibrating and Adjusting**

This chapter explains how to adjust the oscilloscope for optimum operating performance.

## **4 Troubleshooting**

This chapter begins with suggestions for solving general problems that you may encounter with the oscilloscope. Procedures for troubleshooting the oscilloscope follow the problem solving suggestions.

## **5 Replacing Assemblies**

This chapter describes how to remove assemblies from the 2000/3000 X-Series oscilloscope.

## **6 Replaceable Parts**

This chapter describes how to order replaceable assemblies and parts for the Agilent 2000/3000 X-Series oscilloscopes. It includes diagrams and parts lists for hardware that you can order.

## 7 Safety Notices

At the front of the book you will find safety notice descriptions and document warranties.

### **Digital Channels**

Because all of the oscilloscopes in the Agilent 2000/3000 X-Series have analog channels, the analog channel topics in this book apply to all instruments. Whenever a topic discusses the digital channels, that information applies only to Mixed-Signal Oscilloscope (MSO) models or DSO models that have been upgraded to an MSO.

### **Abbreviated instructions for pressing a series of keys**

Instructions for pressing a series of keys are written in an abbreviated manner. Instructions for pressing Key1, then pressing Softkey2, then pressing Softkey3 are abbreviated as follows:

Press [**Key1**] → **Softkey2** → **Softkey3**.

The keys may be front panel keys, or softkeys, which are located directly below the oscilloscope display.



# Contents

	<b>In This Service Guide</b>	<b>3</b>
	<b>Figures</b>	<b>9</b>
	<b>Tables</b>	<b>13</b>
<b>1</b>	<b>Characteristics and Specifications</b>	<b>15</b>
	Power Requirements	16
	Measurement Category	17
	Measurement Category	17
	Measurement Category Definitions	17
	Transient Withstand Capability	18
	Environmental Conditions	19
	Specifications	20
	Contact us	21
<b>2</b>	<b>Testing Performance</b>	<b>23</b>
	Overview	24
	List of Test Equipment	25
	Conventions	26
	To construct the test connector (for use with MSO models only)	27
	To test digital channels (MSO models only)	29
	To verify digital channel threshold accuracy (MSO models only)	30
	When to Test	30

What to Test	30
Verifying Test Results	30
To verify DC vertical gain accuracy	35
To verify dual cursor accuracy	42
To verify bandwidth (-3 dB)	49
To verify time base accuracy	55
To verify trigger sensitivity	57
Test Internal Trigger Sensitivity (all models)	58
Test External Trigger Sensitivity	60
Agilent 2000 X-Series Oscilloscopes Performance Test Record	63
Agilent 3000 X-Series Oscilloscopes Performance Test Record	65
<b>3 Calibrating and Adjusting</b>	<b>67</b>
User Calibration	69
To perform User Cal	69
User Cal Status	72
<b>4 Troubleshooting</b>	<b>73</b>
Solving General Problems with the Oscilloscope	74
If there is no display	74
If there is no trace display	75
If the trace display is unusual or unexpected	75
If you cannot see a channel	76
Verifying Basic Operation	77
To power-on the oscilloscope	77
To perform hardware self test	78
To perform front panel self test	78
To verify default setup	79
To perform an Auto Scale on the Probe Comp signal	80
To compensate passive probes	81

Troubleshooting Internal Assemblies	83
Equipment Required for Troubleshooting Internal Assemblies	83
To prepare for internal assembly troubleshooting	84
Flowchart for Troubleshooting Internal Assemblies	87
System Board Drawings	88
To check the system board power supply test points	90
To check the interboard supply connector voltages	91
To check the line filter board AC output	93
To check the power switch	95
To check the power supply DC output	96
To check the display supplies	97
To check the keyboard supplies	98
To check the fan	99

## 5 Replacing Assemblies 101

To remove the front panel knobs	104
To remove the bucket assembly	105
To remove the power supply shield	107
To remove the rear deck assembly	110
To remove the acquisition board	117
To remove the front panel assembly	122
To remove the display assembly	129
Replacing a 75019-68712 Display Assembly	131
To remove the fan assembly	134
To remove the power supply	136
To remove the line filter board	139

## 6 Replaceable Parts 145

Ordering Replaceable Parts	146
----------------------------	-----

## Contents

Listed Parts	146
Unlisted Parts	146
Direct Mail Order System	146
Exchange Assemblies	147
Exploded Views	148
Replaceable Parts List	150
<b>7 Safety Notices</b>	<b>157</b>
Warnings	157
To clean the instrument	158
Safety Symbols	159
<b>Index</b>	<b>161</b>

## Figures

- Figure 1. Constructing the 8-by-2 Connector 28
- Figure 2. Setting Up Equipment for Digital Channel Threshold Accuracy Test 32
- Figure 3. Setting up Equipment for DC Vertical Gain Accuracy Test 39
- Figure 4. Using a Blocking Capacitor to Reduce Noise 41
- Figure 5. Setting up Equipment for Dual Cursor Accuracy Test 46
- Figure 6. Using a Blocking Capacitor to Reduce Noise 48
- Figure 7. Setting Up Equipment for Bandwidth (-3 dB) Verification Test 51
- Figure 8. Setting Up Equipment for Internal Trigger Sensitivity Test 58
- Figure 9. Setting Up Equipment for 4-Channel External Trigger Sensitivity Test 61
- Figure 10. User Calibration cable for 2-channel oscilloscope 70
- Figure 11. User Calibration cable for 4-channel oscilloscope 71
- Figure 12. Default setup screen 80
- Figure 13. Example pulses 82
- Figure 14. Setup for troubleshooting internal assemblies 85
- Figure 15. System Board Test Points/Connectors - Top Side, Left 88
- Figure 16. System Board Test Points/Connectors - Top Side, Right 89
- Figure 17. Line filter board interboard supply connector J108 92
- Figure 18. Verify line filter board AC output 94
- Figure 19. Verify power switch operation 95
- Figure 20. Location of the Fan Connector 100
- Figure 21. Removing the front panel knobs 104
- Figure 22. Removing the bucket screws 105
- Figure 23. Removing bucket assembly 106

## Figures

- Figure 24. Removing the power supply shield screw 107
- Figure 25. Unclipping the power supply shield right side 108
- Figure 26. Removing the power supply shield - lift and pull out 109
- Figure 27. Removing the BNC nuts and washers 110
- Figure 28. Removing the top rear deck screws 111
- Figure 29. Removing the bottom right rear deck screw 111
- Figure 30. Removing the bottom left rear deck screw 112
- Figure 31. Removing the bottom rear deck screws 112
- Figure 32. Removing the option module guide to acquisition board screw 113
- Figure 33. Disconnecting the interboard supply cable from the acquisition board 114
- Figure 34. Lifting front bezel latch 115
- Figure 35. Separating the rear and front decks 116
- Figure 36. Rear and front decks separated 116
- Figure 37. Removing the T6 screws (4 channel version) 117
- Figure 38. Disconnecting keyboard and display cables from acquisition board 118
- Figure 39. Disconnecting display backlight power cable from acquisition board 119
- Figure 40. Acquisition board mounting screw locations 120
- Figure 41. Acquisition board removed from front deck 121
- Figure 42. Release the bezel clips from the front deck 122
- Figure 43. All bezel clips released 123
- Figure 44. HINT: When reinstalling bezel, align ground terminal first 123
- Figure 45. Gently lift front deck from bezel 124
- Figure 46. Disconnect the keyboard cable 125
- Figure 47. Disconnect the softkey board cable 126
- Figure 48. Unclip the softkey board from the bezel 127
- Figure 49. Remove the softkey keypad from the bezel 127
- Figure 50. Unclip the keyboard board from the bezel 128
- Figure 51. Remove the keyboard keypad from the bezel 128

- Figure 52. Removing the display assembly 129
- Figure 53. Display assembly removed 130
- Figure 54. The 75019-68712 display assembly has a bracket under two of the retaining screws 131
- Figure 55. Disassembling the 75019-68712 display assembly 132
- Figure 56. Separating the 75019-68712 display mounting bracket 133
- Figure 57. Removing the 75019-61606 display cable 133
- Figure 58. Disconnecting fan power cable 134
- Figure 59. Removing fan assembly 135
- Figure 60. Disconnecting the AC cable 136
- Figure 61. Disconnecting the interboard supply cable from the line filter board 137
- Figure 62. Disconnecting the DC cable from the line filter board 137
- Figure 63. Removing the power supply 138
- Figure 64. Removing the option module guide 139
- Figure 65. Disconnecting the ground wire 140
- Figure 66. Removing the line filter board screws 141
- Figure 67. Removing the line filter board 142
- Figure 68. Removing the power switch extender 143
- Figure 69. Exploded View 1 of 2 148
- Figure 70. Exploded View 2 of 2 149


## Figures



## Tables

Table 1. List of test equipment	25
Table 2. Conventions	26
Table 3. Materials required to construct the test connectors	27
Table 4. Equipment Required to Test Digital Channel Threshold Accuracy	31
Table 5. Threshold Accuracy Voltage Test Settings	33
Table 6. DC Vertical Gain Accuracy Test Limits	35
Table 7. Equipment Required to Verify DC Vertical Gain Accuracy	36
Table 8. Settings Used to Verify DC Vertical Gain Accuracy, 2000 X-Series Models	37
Table 9. Settings Used to Verify DC Vertical Gain Accuracy, 3000 X-Series Models	38
Table 10. Equipment Required to Verify Dual Cursor Accuracy	43
Table 11. Settings Used to Verify Dual Cursor Accuracy, 2000 X-Series Models	44
Table 12. Settings Used to Verify Dual Cursor Accuracy, 3000 X-Series Models	45
Table 13. Bandwidth (-3 dB) Test Limits	49
Table 14. Equipment Required to Verify Bandwidth (-3 dB)	50
Table 15. Equipment Required to Verify Time Base Accuracy	55
Table 16. Equipment Required to Verify Trigger Sensitivity	57
Table 17. Equipment Required to Troubleshoot the Oscilloscope	83
Table 18. Replaceable Parts	150

## Tables

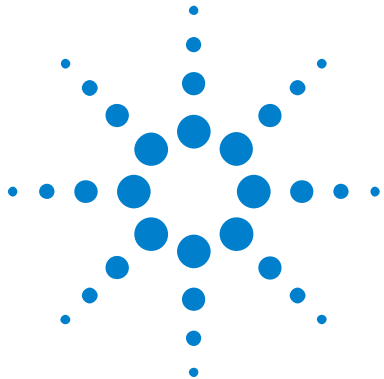

# 1 Characteristics and Specifications

Power Requirements	16
Measurement Category	17
Environmental Conditions	19
Specifications	20
Contact us	21

This chapter contains a partial list of characteristics and specifications for the Agilent InfiniiVision 2000/3000 X-Series oscilloscopes.

For a full list of Agilent InfiniiVision 2000/3000 X-Series oscilloscopes characteristics and specifications see the data sheets.

The data sheets are available at  
[www.agilent.com/find/2000X-Series](http://www.agilent.com/find/2000X-Series) or  
[www.agilent.com/find/3000X-Series](http://www.agilent.com/find/3000X-Series).



## Power Requirements

Line voltage, frequency, and power:

- ~Line 100-120 Vac, 50/60/400 Hz
- 100-240 Vac, 50/60 Hz
- 100 W max

## Measurement Category

### Measurement Category

The InfiniiVision 2000/3000 X-Series oscilloscope is intended to be used for measurements in Measurement Category I.

**WARNING**

**Use this instrument only for measurements within its specified measurement category.**

---

### Measurement Category Definitions

Measurement category I is for measurements performed on circuits not directly connected to MAINS. Examples are measurements on circuits not derived from MAINS, and specially protected (internal) MAINS derived circuits. In the latter case, transient stresses are variable; for that reason, the transient withstand capability of the equipment is made known to the user.

Measurement category II is for measurements performed on circuits directly connected to the low voltage installation. Examples are measurements on household appliances, portable tools and similar equipment.

Measurement category III is for measurements performed in the building installation. Examples are measurements on distribution boards, circuit-breakers, wiring, including cables, bus-bars, junction boxes, switches, socket-outlets in the fixed installation, and equipment for industrial use and some other equipment, for example, stationary motors with permanent connection to the fixed installation.

Measurement category IV is for measurements performed at the source of the low-voltage installation. Examples are electricity meters and measurements on primary overcurrent protection devices and ripple control units.

## Transient Withstand Capability

### CAUTION

Maximum input voltage for analog inputs  
CAT I 300 Vrms, 400 Vpk; transient overvoltage 1.6 kVpk  
with 10073C 10:1 probe: CAT I 500 Vpk, CAT II 400 Vpk  
with N2862A/B or N2863A/B 10:1 probe: 300 Vrms

---

### CAUTION

Do not exceed 5 Vrms in 50  $\Omega$  mode (3000 X-Series oscilloscopes only). Input protection is enabled in 50  $\Omega$  mode, and the 50  $\Omega$  load will disconnect if greater than 5 Vrms is detected. However, the input could still be damaged, depending on the time constant of the signal. The 50  $\Omega$  input protection mode only functions when the oscilloscope is powered on.

---

### CAUTION

Maximum input voltage for logic channels:  
 $\pm 40$  V peak CAT I; transient overvoltage 800 Vpk

---

## Environmental Conditions

Environment	Indoor use only.
Ambient temperature	Operating 0 °C to +55 °C; non-operating –40 °C to +71 °C
Humidity	Operating: Up to 80% RH at or below +40 °C. Up to 45% RH up to +50 °C. Non-operating: Up to 95% RH up to +40 °C. Up to 45% RH up to +50 °C.
Altitude	Operating and non-operating to 4,000 m (13,123 ft)
Overvoltage Category	This product is intended to be powered by MAINS that comply to Overvoltage Category II, which is typical of cord-and-plug connected equipment.
Pollution Degree	The InfiniiVision 2000/3000 X-Series oscilloscopes may be operated in environments of Pollution Degree 2 (or Pollution Degree 1).
Pollution Degree Definitions	<p>Pollution Degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence. Example: A clean room or climate controlled office environment.</p> <p>Pollution Degree 2. Normally only dry non-conductive pollution occurs. Occasionally a temporary conductivity caused by condensation may occur. Example: General indoor environment.</p> <p>Pollution Degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. Example: Sheltered outdoor environment.</p>

## Specifications

Please see the *InfiniiVision 2000/3000 X-Series Oscilloscopes Data Sheet* for complete, up-to-date specifications and characteristics.

To download a copy of the data sheet please visit:

[www.agilent.com/find/2000X-Series](http://www.agilent.com/find/2000X-Series) or

[www.agilent.com/find/3000X-Series](http://www.agilent.com/find/3000X-Series).

Or go to the Agilent home page at [www.agilent.com](http://www.agilent.com) and search for **2000/3000 X-Series oscilloscopes data sheet**.

To order a data sheet by phone, please contact your local Agilent office. A contact list is provided on the next page. The most up-to-date list is available at:

[www.agilent.com/find/contactus](http://www.agilent.com/find/contactus)



## Contact us

### Americas

Canada (877) 894-4414  
Latin America 305 269 7500  
United States (800) 829-4444

### Asia Pacific

Australia 1 800 629 485  
China 800 810 0189  
Hong Kong 800 938 693  
India 1 800 112 929  
Japan 81 426 56 7832  
Korea 080 769 0800  
Malaysia 1 800 888 848  
Singapore 1 800 375 8100  
Taiwan 0800 047 866  
Thailand 1 800 226 008

### Europe

Austria 0820 87 44 11  
Belgium 32 (0) 2 404 93 40  
Denmark 45 70 13 15 15  
Finland 358 (0) 10 855 2100  
France 0825 010 700  
Germany 01805 24 6333\*  
\*0.14€/minute  
Ireland 1890 924 204  
Italy 39 02 92 60 8484  
Netherlands 31 (0) 20 547 2111  
Spain 34 (91) 631 3300  
Sweden 0200-88 22 55  
Switzerland (French)  
44 (21) 8113811 (Opt 2)  
Switzerland (German)  
0800 80 53 53 (Opt 1)  
United Kingdom 44 (0) 7004 666666  
Other European countries:  
[www.agilent.com/find/contactus](http://www.agilent.com/find/contactus)

## **1 Characteristics and Specifications**



## 2 Testing Performance

Overview	24
List of Test Equipment	25
To construct the test connector (for use with MSO models only)	27
To test digital channels (MSO models only)	29
To verify digital channel threshold accuracy (MSO models only)	30
To verify DC vertical gain accuracy	35
To verify dual cursor accuracy	42
To verify bandwidth (-3 dB)	49
To verify time base accuracy	55
To verify trigger sensitivity	57
Agilent 2000 X-Series Oscilloscopes Performance Test Record	63
Agilent 3000 X-Series Oscilloscopes Performance Test Record	65

This chapter explains how to verify correct oscilloscope operation and perform tests to ensure that the oscilloscope meets the performance specifications.



# Overview

To completely test and troubleshoot MSO models, create and use the test connector accessory as described in this chapter.

- The test connector is only required for oscilloscopes that have the MSO option licensed (enabled).
- The connector is used in the digital channel threshold accuracy test.
- The test connector keeps electrical distortion to a minimum and makes it easy for you to connect the oscilloscope probes to function generators and measurement equipment.

### Let the Equipment Warm Up Before Testing

For accurate test results, let the test equipment and the oscilloscope warm up 30 minutes before testing.

### Verifying Test Results

During the tests, record the readings in the Performance Test Record on [page 63](#). To verify whether a test passes, verify that the reading is within the limits in the Performance Test Record.

**If a performance test fails**

If a performance test fails, first perform the User Cal procedure. Press the following keys to access User Cal: [Utility]→Service→Start User Cal.

## List of Test Equipment

Below is a list of test equipment and accessories required to perform the performance test verification procedures.

**Table 1** List of test equipment

Equipment	Critical Specifications	Recommended Model/ Part Number
Test connector, 8-by-2*	See <a href="#">page 27</a> for instructions on building test connector.	n/a
Digital Multimeter	0.1 mV resolution, 0.005% accuracy	Agilent 34401A
Power Splitter	Outputs differ by 0.15 dB	Agilent 11667B
Oscilloscope Calibrator	DC offset voltage of -5.5 V to 35.5 V, 0.1 V resolution 25 MHz—500 MHz sine wave, 5 ppm	Fluke 5820A
Signal Generator	25 MHz, 100 MHz, 350 MHz, 500 MHz, and 1 GHz sine waves	Agilent N5181A
Power Meter	1 GHz $\pm 3\%$ accuracy	Agilent N1914A
Power Sensor	1 GHz $\pm 3\%$ accuracy	Agilent E9304A or N8482A
BNC banana cable	BNC (m) to dual banana	Pomona 2BC-BNC-36 or Agilent 11001-66001
BNC cable (qty 3)	BNC - BNC, 48" length	Agilent 10503A <sup>†</sup>
Cable	Type N (m) 609.6 mm (24 in.)	Agilent 11500B
Probe cable*	No substitute	Agilent N6450-60001 (16-channel) or Agilent N6459-60001 (8-channel) <sup>†</sup>
Adapter	BNC(f) to banana(m)	Agilent 1251-2277 <sup>†</sup>
Adapter	BNC Tee (m) (f) (f)	Agilent 1250-0781 <sup>†</sup> or Pomona 3285

\* Required only for testing digital channels of oscilloscopes that have the MSO option.

Most parts and equipment are available at [www.agilent.com](http://www.agilent.com). See respective manufacturer's websites for their equipment.

<sup>†</sup> These parts available at [www.parts.agilent.com](http://www.parts.agilent.com) at the time this manual was published.

## 2 Testing Performance

**Table 1** List of test equipment (continued)

Equipment	Critical Specifications	Recommended Model/ Part Number
Adapter	Type N (m) to BNC (m)	Agilent 1250-0082 or Pomona 3288 with Pomona 3533
Blocking capacitor and shorting cap	Note: if a BNC blocking capacitor is not available use an SMA blocking capacitor.	Agilent 11742A + Pomona 4288 + Pomona 5088
Adapter (qty 3)	N(m) to BNC(f)	Agilent 1250-0780
50 Ohm Feedthrough Termination	50Ω BNC (f) to BNC (m)	Agilent 0960-0301

\* Required only for testing digital channels of oscilloscopes that have the MSO option.  
 † Most parts and equipment are available at [www.agilent.com](http://www.agilent.com). See respective manufacturer's websites for their equipment.  
 † These parts available at [www.parts.agilent.com](http://www.parts.agilent.com) at the time this manual was published.

## Conventions

The following conventions will be used when referring to oscilloscope models throughout this chapter.

**Table 2** Conventions

Models	Referred to as:
MSO-X /DSO-X 2002A, MSO-X /DSO-X 2004A	70 MHz Models
MSO-X /DSO-X 2012A, MSO-X /DSO-X 2014A MSO-X /DSO-X 3012A, MSO-X /DSO-X 3014A	100 MHz Models
MSO-X /DSO-X 2022A, MSO-X /DSO-X 2024A MSO-X /DSO-X 3024A	200 MHz Models
MSO-X /DSO-X 3032A, MSO-X /DSO-X 3034A	350 MHz Models
MSO-X /DSO-X 3052A, MSO-X /DSO-X 3054A	500 MHz Models
MSO-X /DSO-X 3102A, MSO-X /DSO-X 3104A	1 GHz Models


## To construct the test connector (for use with MSO models only)

Agilent 2000/3000 X-Series oscilloscopes that have digital channels enabled require the test connector described below. Follow the steps to build the test connector.

**Table 3** Materials required to construct the test connectors

Description	Recommended Part	Qty
BNC (f) Connector	Agilent 1250-1032 or Pomona 4578	1
Berg Strip, 8-by-2	3M .100" x .100" Pin Strip Header or similar	1 strip, cut to length (8x2)
Jumper wire		

- 1** Obtain a BNC connector and an 8-by-2 section of Berg strip. A longer strip can be cut to length using wire cutters.
- 2** On one side of the Berg strip, solder a jumper wire to all of the pins (shown in [Figure 1](#) on page 28).
- 3** On the other side of the Berg strip, solder another jumper wire to all of the pins.
- 4** Solder the center of the BNC connector to a center pin on one of the rows on the Berg strip.
- 5** Solder the ground tab of the BNC connector to a center pin on the other row on the Berg strip.

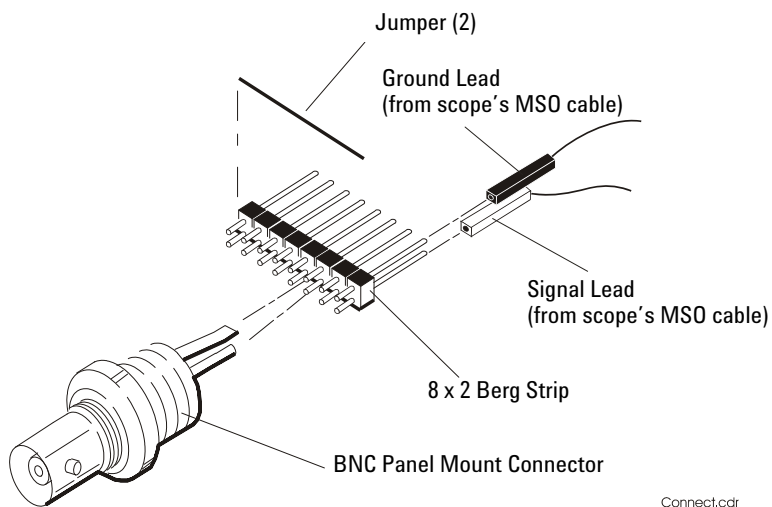

Connect.cdr

**Figure 1** Constructing the 8-by-2 Connector



## To test digital channels (MSO models only)

The acquisition system testing provides confidence that the acquisition system is functioning correctly. It does not, however, check a particular specification.

- 1 Disconnect all probes from the circuit under test and from any other input source.
- 2 Using probe leads and grabbers, connect digital channels D0, D1, D2, and D3 to the Probe Comp signal on the center of the front panel.
- 3 Press the [**AutoScale**] key.

If four square waves appear, the acquisition system is functioning correctly.

If the square waves do not appear, go to the “Troubleshooting” chapter. Then return here to finish testing the digital channels.

- 4 Disconnect the digital channels from the calibration point.
- 5 Use steps 2 and 3 to test the following sets of digital channels. After you test one set of digital channels, remove them before connecting the next set.
  - D4, D5, D6, D7
  - D8, D9, D10, D11 (on 3000 X-Series models)
  - D12, D13, D14, D15 (on 3000 X-Series models)

## To verify digital channel threshold accuracy (MSO models only)

This test verifies the digital channel threshold accuracy specification of the Agilent 2000/3000 X-Series oscilloscopes.

Threshold accuracy test limits:  $\pm(100 \text{ mV} + 3\% \text{ of threshold setting})$

### When to Test

You should perform this test every 12 months or after 2000 hours of operation, whichever comes first.

### What to Test

Use these instructions to test the threshold settings of digital channels D7-D0. Then, use the same instructions to test digital channels D15-D8 (on 3000 X-Series).

### Verifying Test Results


After each threshold test, record the voltage reading in the Performance Test Record on [page 63](#). To verify whether a test passes, verify that the voltage reading is within the limits in the Performance Test Record.

**Table 4** Equipment Required to Test Digital Channel Threshold Accuracy

Equipment	Critical Specifications	Recommended Model/Part
Digital Multimeter	0.1 mV resolution, 0.005% accuracy	Agilent 34401A
Oscilloscope Calibrator	DC offset voltage 6.3 V	Fluke 5820A
BNC-Banana Cable		Agilent 11001-66001 or Pomona 2BC-BNC-36
BNC Tee		Agilent 1250-0781 or Pomona 3285
50 $\Omega$ BNC Cable		Agilent 10503A
BNC Test Connector, 8-by-2		User-built (See <a href="#">page 27</a> )
Probe Cable		Agilent N6450-60001 (16-channel) or Agilent N6459-60001 (8-channel)

- 1** Turn on the test equipment and the oscilloscope. Let them warm up for 30 minutes before starting the test.
- 2** Set up the oscilloscope calibrator.
  - a** Set the oscilloscope calibrator to provide a DC offset voltage at the Channel 1 output.
  - b** Use the multimeter to monitor the oscilloscope calibrator DC output voltage.
- 3** Use the 8-by-2 test connector and the BNC cable assembly to connect digital channels D0-D7 to one side of the BNC Tee. Then connect the D0-D7 ground lead to the ground side of the 8-by-2 connector. See [Figure 2](#).

## 2 Testing Performance

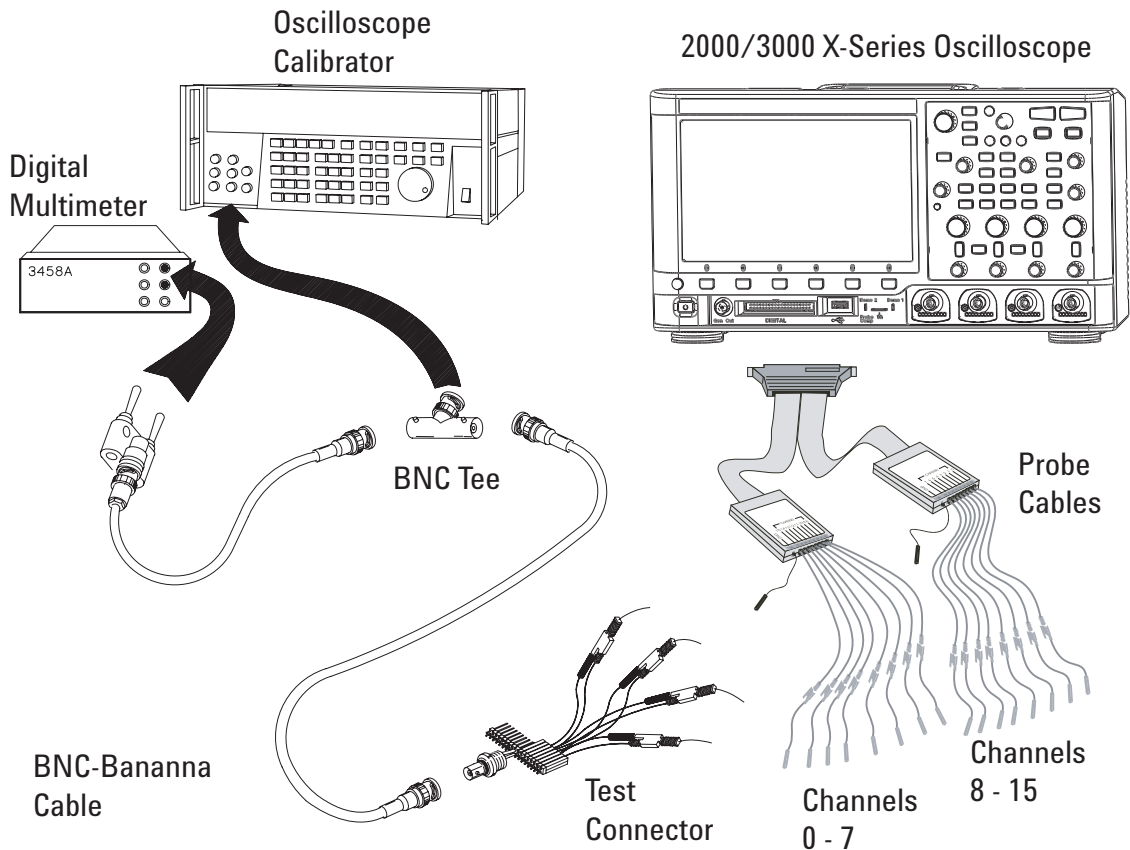

**Figure 2** Setting Up Equipment for Digital Channel Threshold Accuracy Test

- 4 Use a BNC-banana cable to connect the multimeter to the other side of the BNC Tee.
- 5 Connect the BNC Tee to the Channel 1 output of the calibrator as shown in Figure 2.
- 6 On the oscilloscope, press the **[Digital]** key, then press the **Thresholds** softkey, then press the **D7 - D0** softkey repeatedly until the check mark is next to **User**.
- 7 Press the **User** softkey to the right of the **D7 - D0** softkey, then turn the Entry knob (↻) on the front panel of the

oscilloscope to set the threshold test settings as shown in [Table 5](#).

**Table 5** Threshold Accuracy Voltage Test Settings

Threshold voltage setting (in oscilloscope User softkey)	DC offset voltage setting (on oscilloscope calibrator)	Limits
+5.00 V	+5.250 V $\pm$ 1 mV dc	Lower limit = +4.750 V Upper limit = +5.250 V
-5.00 V	-4.750 V $\pm$ 1 mV dc	Lower limit = -5.250 V Upper limit = -4.750 V
0.00 V	+100m V $\pm$ 1 mV dc	Upper limit = +100 mV Lower limit = -100 mV

**8** Do the following steps for each of the threshold voltage levels shown in [Table 5](#).

- a** Set the threshold voltage shown in the **User** softkey using the Entry knob on the oscilloscope.
- b** Enter the corresponding DC offset voltage on the oscilloscope calibrator front panel. Then use the multimeter to verify the voltage.

Digital channel activity indicators are displayed on the status line at the top of the oscilloscope display. The activity indicators for D7-D0 should show all of the channels at digital high levels.

- c** Use the knob on the oscilloscope calibrator to decrease the offset voltage, in increments of 10 mV, until the activity indicators for digital channels D7-D0 are all at digital low levels. Record the oscilloscope calibrator voltage in the Performance Test Record (see [page 63](#)).
- d** Use the knob on the oscilloscope calibrator to increase the offset voltage, in increments of 10 mV, until the activity indicators for digital channels D7-D0 are all at digital high levels. Record the oscilloscope calibrator voltage in the Performance Test Record (see [page 63](#)).

Before proceeding to the next step, make sure that you have recorded the oscilloscope calibrator voltage levels for each of the threshold settings shown in [Table 5](#).

- 9** When testing 3000 X-Series MSOs, use the 8-by-2 test connector to connect digital channels D15-D8 to the output of the oscilloscope calibrator. Then connect the D15-D8 ground lead to the ground side of the 8-by-2 connector.
- 10** Repeat this procedure (steps 6 through 8) for digital channels D15-D8 to verify threshold accuracy and record the threshold levels in the Performance Test Record (see [page 63](#)). Be sure to set the thresholds with the **User** softkey for the appropriate set of channels.

## To verify DC vertical gain accuracy

This test verifies the accuracy of the analog channel DC vertical gain for each channel.

In this test, you will measure the dc voltage output of an oscilloscope calibrator using the oscilloscope's


**Average - Full Screen** voltage measurement and compare the results with the multimeter reading.

**Table 6** DC Vertical Gain Accuracy Test Limits

Models	Test Limits	Notes
2000 X-Series	±3% of full scale ( $\geq 10$ mV/div); ±4% of full scale ( $< 10$ mV/div)	<ul style="list-style-type: none"> <li>Full scale is defined as 32 mV on the 2 mV/div range and the 1 mV/div range.</li> </ul>
3000 X-Series	±2.0% of full scale	<ul style="list-style-type: none"> <li>Full scale on all other ranges is defined as 8 divisions times the V/div setting.</li> </ul>

**Table 7** Equipment Required to Verify DC Vertical Gain Accuracy

Equipment	Critical Specifications	Recommended Model/Part
Oscilloscope Calibrator	14 mV to 35 Vdc, 0.1 V resolution	Fluke 5820A
Digital multimeter	Better than 0.01% accuracy	Agilent 34401A
Cable	BNC, Qty 2	Agilent 10503A
Shorting cap	BNC	Agilent 1250-0774
Adapter	BNC (f) to banana (m)	Agilent 1251-2277
Adapter	BNC tee (m) (f) (f)	Agilent 1250-0781 or Pomona 3285
Blocking capacitor		Agilent 11742A + Pomona 4288 + Pomona 5088

- 1 Press **[Save/Recall] > Default/Erase > Factory Default** to recall the factory default setup.
- 2 If you are testing a 2000 X-Series oscilloscope, set the probe attenuation to 1:1 on the analog channel you are testing (for example, **[1] > Probe > Probe**; then, turn the  Entry knob to select **1.00 : 1**).
- 3 Set up the oscilloscope.
  - a Adjust the horizontal scale to **10.00 ms/div**.
  - b Set the Volts/Div setting to the value in the first line in [Table 8](#) or [Table 9](#) (depending on the oscilloscope model).
  - c Adjust the channel's vertical position knob to place the baseline (reference level) at 0.5 major division from the bottom of the display.



**Table 8** Settings Used to Verify DC Vertical Gain Accuracy, 2000 X-Series Models

Volts/Div Setting	Oscilloscope Calibrator Setting	Test Limits		
5 V/Div	35 V	33.8 V	to	36.2 V
2 V/Div	14 V	13.52 V	to	14.48 V
1 V/Div	7 V	6.76 V	to	7.24 V
500 mV/Div	3.5 V	3.38 V	to	3.62 V
200 mV/Div	1.4 V	1.352 V	to	1.448 V
100 mV/Div	700 mV	676 mV	to	724 mV
50 mV/Div	350 mV	338 mV	to	362 mV
20 mV/Div	140 mV	135.2 mV	to	144.8 mV
10 mV/Div	70 mV	67.6 mV	to	72.4 mV
5 mV/Div <sup>1</sup>	35 mV	33.4 mV	to	36.6 mV
2 mV/Div <sup>1,2</sup>	14 mV	12.72 mV	to	15.28 mV
1 mV/Div <sup>1,2</sup>	7 mV	5.72 mV	to	8.28 mV

<sup>1</sup> A blocking capacitor is required at this range to reduce noise. See [“Use a Blocking Capacitor to Reduce Noise”](#) on page 41.


<sup>2</sup> Full scale is defined as 32 mV on the 2 mV/div and the 1 mV/div range. Full scale on all other ranges is defined as 8 divisions times the V/div setting.

**Table 9** Settings Used to Verify DC Vertical Gain Accuracy, 3000 X-Series Models


Volts/Div Setting	Oscilloscope Calibrator Setting	Test Limits		
5 V/Div	35 V	34.2 V	to	35.8 V
2 V/Div	14 V	13.68 V	to	14.32 V
1 V/Div	7 V	6.84 V	to	7.16 V
500 mV/Div	3.5 V	3.42 V	to	3.58 V
200 mV/Div	1.4 V	1.368 V	to	1.432 V
100 mV/Div	700 mV	684 mV	to	716 mV
50 mV/Div	350 mV	342 mV	to	358 mV
20 mV/Div	140 mV	136.8 mV	to	143.2 mV
10 mV/Div	70 mV	68.4 mV	to	71.6 mV
5 mV/Div <sup>1</sup>	35 mV	34.2 mV	to	35.8 mV
2 mV/Div <sup>1,2</sup>	14 mV	13.36 mV	to	14.64 mV
1 mV/Div <sup>1,2</sup>	7 mV	6.36 mV	to	7.64 mV

<sup>1</sup> A blocking capacitor is required at this range to reduce noise. See [“Use a Blocking Capacitor to Reduce Noise”](#) on page 41.

<sup>2</sup> Full scale is defined as 32 mV on the 2 mV/div range and the 1 mV/div range. Full scale on all other ranges is defined as 8 divisions times the V/div setting.

- d** Press the **[Acquire]** key.
  - e** Then press the **Acq Mode** softkey and select **Averaging**.
  - f** Then press the **#Avgs** softkey and set it to 64.
- Wait a few seconds for the measurement to settle.
- 4** Add a measurement for the average voltage:
    - a** Press the **[Meas]** key.
    - b** Press **Source**; then, turn the Entry knob (labeled  on the front panel) to select the channel you are testing.

- c Press **Type**; then, turn the Entry knob to select **Average - Full Screen**, and press **Add Measurement**.
- 5 Read the “current” average voltage value as  $V_1$ .
- 6 Use the BNC tee and cables to connect the oscilloscope calibrator /power supply to both the oscilloscope and the multimeter (see [Figure 3](#)).

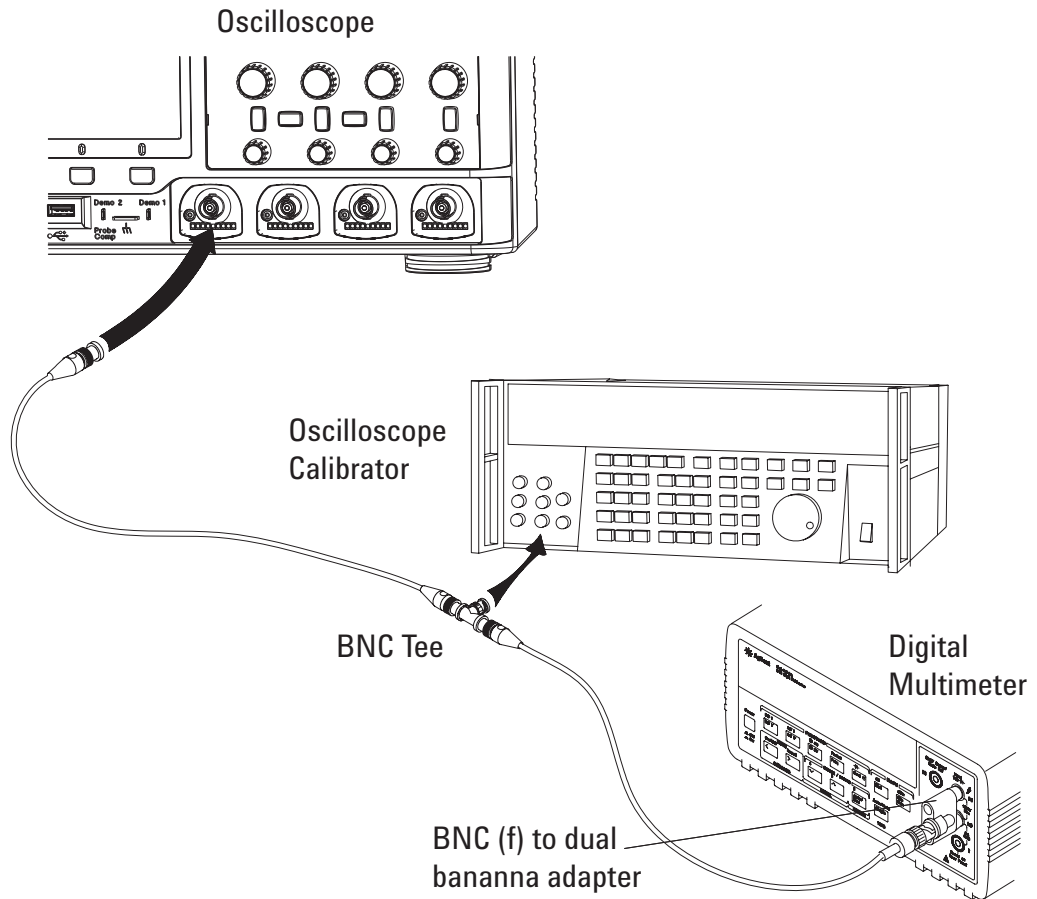

**Figure 3** Setting up Equipment for DC Vertical Gain Accuracy Test

- 7 Adjust the output so that the multimeter reading displays the first Volts/div calibrator setting value in [Table 8](#) or [Table 9](#) (depending on the oscilloscope model).
- 8 Disconnect the multimeter.
- 9 Wait until the measurement settles.
- 10 Read the “current” average voltage value again as V2.
- 11 Calculate the difference  $V2 - V1$ .


The difference in average voltage readings should be within the test limits of [Table 8](#) or [Table 9](#) (depending on the oscilloscope model).

If a result is not within the test limits, go to the “Troubleshooting” chapter. Then return here.

- 12 Disconnect the oscilloscope calibrator from the oscilloscope.
- 13 Repeat this procedure to check the DC vertical gain accuracy with the remaining Volts/div setting values in [Table 8](#) or [Table 9](#) (depending on the oscilloscope model).
- 14 Finally, repeat this procedure for the remaining channels to be tested.

### Use a Blocking Capacitor to Reduce Noise

On the more sensitive ranges, such as 1 mV/div, 2 mV/div, and 5 mV/div, noise may be a factor. To eliminate the noise, add a BNC Tee, blocking capacitor, and shorting cap at the oscilloscope channel input to shunt the noise to ground. See [Figure 4](#). If a BNC capacitor is not available, use an SMA blocking capacitor, adapter, and cap. See [“Blocking capacitor and shorting cap”](#) in the equipment list on [page 26](#) for details.

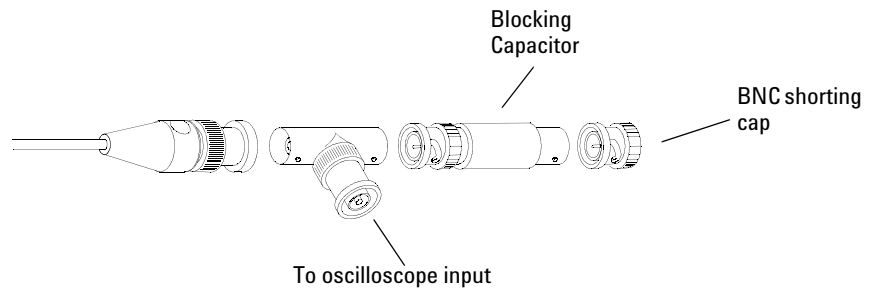

**Figure 4** Using a Blocking Capacitor to Reduce Noise

## To verify dual cursor accuracy

This test verifies the dual cursor accuracy for each analog channel.


This test is similar to the test for verifying the DC vertical gain, except you will measure the dc voltage output of an oscilloscope calibrator using dual cursors on the oscilloscope and compare the results with the multimeter reading.

Dual cursor accuracy test limits:  $\pm$ [DC vertical gain accuracy + 0.5% full scale]

For the DC vertical gain accuracy test limits, see [Table 6](#) on page 35.

**Table 10** Equipment Required to Verify Dual Cursor Accuracy

Equipment	Critical Specifications	Recommended Model/Part
Oscilloscope Calibrator	14 mV to 35 Vdc, 0.1 V resolution	Fluke 5820A
Digital multimeter	Better than 0.01% accuracy	Agilent 34401A
Cable	BNC, Qty 2	Agilent 10503A
Shorting cap	BNC	Agilent 1250-0774
Adapter	BNC (f) to banana (m)	Agilent 1251-2277
Adapter	BNC tee (m) (f) (f)	Agilent 1250-0781 or Pomona 3285
Blocking capacitor		Agilent 11742A + Pomona 4288 + Pomona 5088

- 1 Press **[Save/Recall] > Default/Erse > Factory Default** to recall the factory default setup.
- 2 If you are testing a 2000 X-Series oscilloscope, set the probe attenuation to 1:1 on the analog channel you are testing (for example, **[1] > Probe > Probe**; then, turn the  Entry knob to select **1.00 : 1**).
- 3 Set up the oscilloscope.
  - a Set the Volts/Div setting to the value in the first line in [Table 11](#) or [Table 12](#) (depending on the oscilloscope model).
  - b Adjust the channel 1 position knob to place the baseline at 0.5 major division from the bottom of the display.

**Table 11** Settings Used to Verify Dual Cursor Accuracy, 2000 X-Series Models

Volts/Div Setting	Oscilloscope Calibrator Setting	Test Limits		
5 V/Div	35 V	33.6 V	to	36.4 V
2 V/Div	14 V	13.44 V	to	14.56 V
1 V/Div	7 V	6.72 V	to	7.28 V
500 mV/Div	3.5 V	3.36 V	to	3.64 V
200 mV/Div	1.4 V	1.344 V	to	1.456 V
100 mV/Div	700 mV	672 mV	to	728 mV
50 mV/Div	350 mV	336 mV	to	364 mV
20 mV/Div	140 mV	134.4 mV	to	145.6 mV
10 mV/Div	70 mV	67.2 mV	to	72.8 mV
5 mV/Div <sup>1</sup>	35 mV	33.2 mV	to	36.8 mV
2 mV/Div <sup>1,2</sup>	14 mV	12.56 mV	to	15.44 mV
1 mV/Div <sup>1,2</sup>	7 mV	5.56 mV	to	8.44 mV

<sup>1</sup> A blocking capacitor is required at this range to reduce noise. See [“Use a Blocking Capacitor to Reduce Noise”](#) on page 48.

<sup>2</sup> Full scale is defined as 32 mV on the 2 mV/div range and the 1 mV/div range. Full scale on all other ranges is defined as 8 divisions times the V/div setting.



**Table 12** Settings Used to Verify Dual Cursor Accuracy, 3000 X-Series Models


Volts/Div Setting	Oscilloscope Calibrator Setting	Test Limits		
5 V/Div	35 V	34.0 V	to	36.0 V
2 V/Div	14 V	13.6 V	to	14.4 V
1 V/Div	7 V	6.8 V	to	7.2 V
500 mV/Div	3.5 V	3.4 V	to	3.6 V
200 mV/Div	1.4 V	1.36 V	to	1.44 V
100 mV/Div	700 mV	680 mV	to	720 mV
50 mV/Div	350 mV	340 mV	to	360 mV
20 mV/Div	140 mV	136 mV	to	144 mV
10 mV/Div	70 mV	68 mV	to	72 mV
5 mV/Div <sup>1</sup>	35 mV	34 mV	to	36 mV
2 mV/Div <sup>1,2</sup>	14 mV	13.2 mV	to	14.8 mV
1 mV/Div <sup>1,2</sup>	7 mV	6.2 mV	to	7.8 mV

<sup>1</sup> A blocking capacitor is required at this range to reduce noise. See [“Use a Blocking Capacitor to Reduce Noise”](#) on page 48.


<sup>2</sup> Full scale is defined as 32 mV on the 2 mV/div range and the 1 mV/div range. Full scale on all other ranges is defined as 8 divisions times the V/div setting.

- c** Press the **[Acquire]** key.
- d** Then press the **Acq Mode** softkey and select **Averaging**.
- e** Then press the **#Avgs** softkey and set it to 64.

Wait a few seconds for the measurement to settle.

- 4** Press the **[Cursors]** key, set the **Mode** softkey to **Normal**, then press the **XY** softkey and select **Y**. Press the **Y1** softkey, then use the Entry knob (labeled  on the front panel) to set the Y1 cursor on the baseline of the signal.

- 5 Use the BNC tee and cables to connect the oscilloscope calibrator /power supply to both the oscilloscope and the multimeter (see [Figure 5](#)).

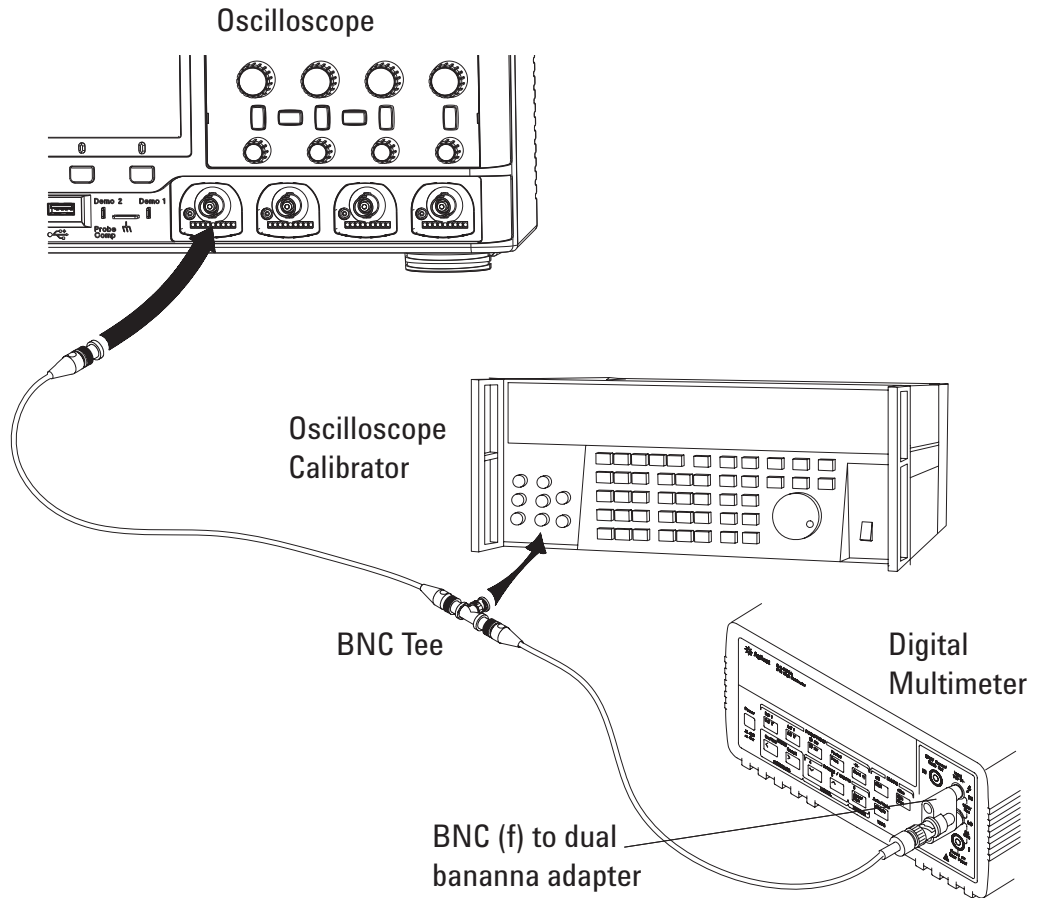

**Figure 5** Setting up Equipment for Dual Cursor Accuracy Test

- 6 Adjust the output so that the multimeter reading displays the first Volts/div calibrator setting value in [Table 11](#) or [Table 12](#) (depending on the oscilloscope model).
- 7 Disconnect the multimeter.
- 8 Wait until the measurement settles.

- 9 Press the **Y2** softkey, then position the Y2 cursor to the center of the voltage trace using the Entry knob.


The  $\Delta Y$  value on the lower line of the display should be within the test limits of [Table 11](#) or [Table 12](#) (depending on the oscilloscope model).

If a result is not within the test limits, go to the “Troubleshooting” chapter. Then return here.

- 10 Disconnect the oscilloscope calibrator from the oscilloscope.
- 11 Repeat this procedure to check the dual cursor accuracy with the remaining Volts/div setting values in [Table 11](#) or [Table 12](#) (depending on the oscilloscope model).
- 12 Finally, repeat this procedure for the remaining channels to be tested.

### Use a Blocking Capacitor to Reduce Noise

On the more sensitive ranges, such as 1 mV/div, 2 mV/div, and 5 mV/div, noise may be a factor. To eliminate the noise, add a BNC Tee, blocking capacitor, and shorting cap at the oscilloscope channel input to shunt the noise to ground. See [Figure 6](#). If a BNC capacitor is not available, use an SMA blocking capacitor, adapter, and cap. See [“Blocking capacitor and shorting cap”](#) in the equipment list on [page 26](#) for details.

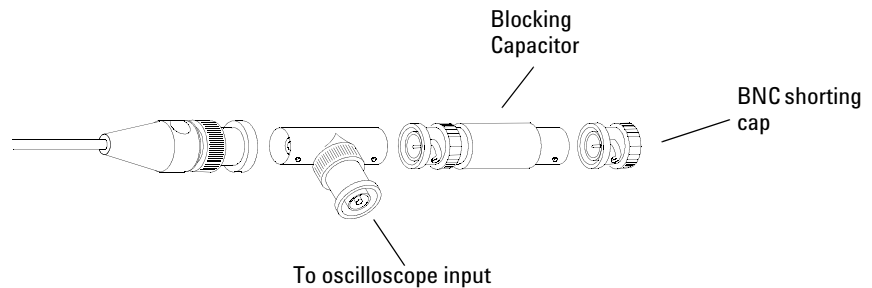

**Figure 6** Using a Blocking Capacitor to Reduce Noise

## To verify bandwidth (-3 dB)

This test checks the bandwidth (-3 dB) of the oscilloscope. In this test you will use a signal generator and a power meter.


**Table 13** Bandwidth (-3 dB) Test Limits

<b>Models</b>	<b>Test Limits</b>
1 GHz Models	All channels (-3 dB), dc to 1 GHz
500 MHz Models	All channels (-3 dB), dc to 500 MHz
350 MHz Models	All channels (-3 dB), dc to 350 MHz
200 MHz Models	All channels (-3 dB), dc to 200 MHz
100 MHz Models	All channels (-3 dB), dc to 100 MHz
70 MHz Models	All channels (-3 dB), dc to 70 MHz

**Table 14** Equipment Required to Verify Bandwidth (-3 dB)

Equipment	Critical Specifications	Recommended Model/Part
Signal Generator	100 kHz - 1 GHz at 200 mVrms	Agilent N5181A
Power Meter	1 MHz - 1 GHz $\pm 3\%$ accuracy	Agilent N1914A
Power Sensor	1 MHz - 1 GHz $\pm 3\%$ accuracy	Agilent E9304A or N8482A
Power Splitter	outputs differ by $< 0.15$ dB	Agilent 11667A
Cable	Type N (m) 24 inch	Agilent 11500B
Adapter	Type N (m) to BNC (m)	Agilent 1250-0082 or Pomona 3288 with Pomona 3533
50 Ohm Feedthrough Termination	50 $\Omega$ BNC (f) to BNC (m), when testing 2000 X-Series oscilloscopes	Agilent 0960-0301

- 1 Connect the equipment (see [Figure 7](#)).
  - a Use the N cable to connect the signal generator to the input of the power splitter input.
  - b Connect the power sensor to one output of the power splitter.
  - c Use an N-to-BNC adapter to connect the other splitter output to the channel 1 input.

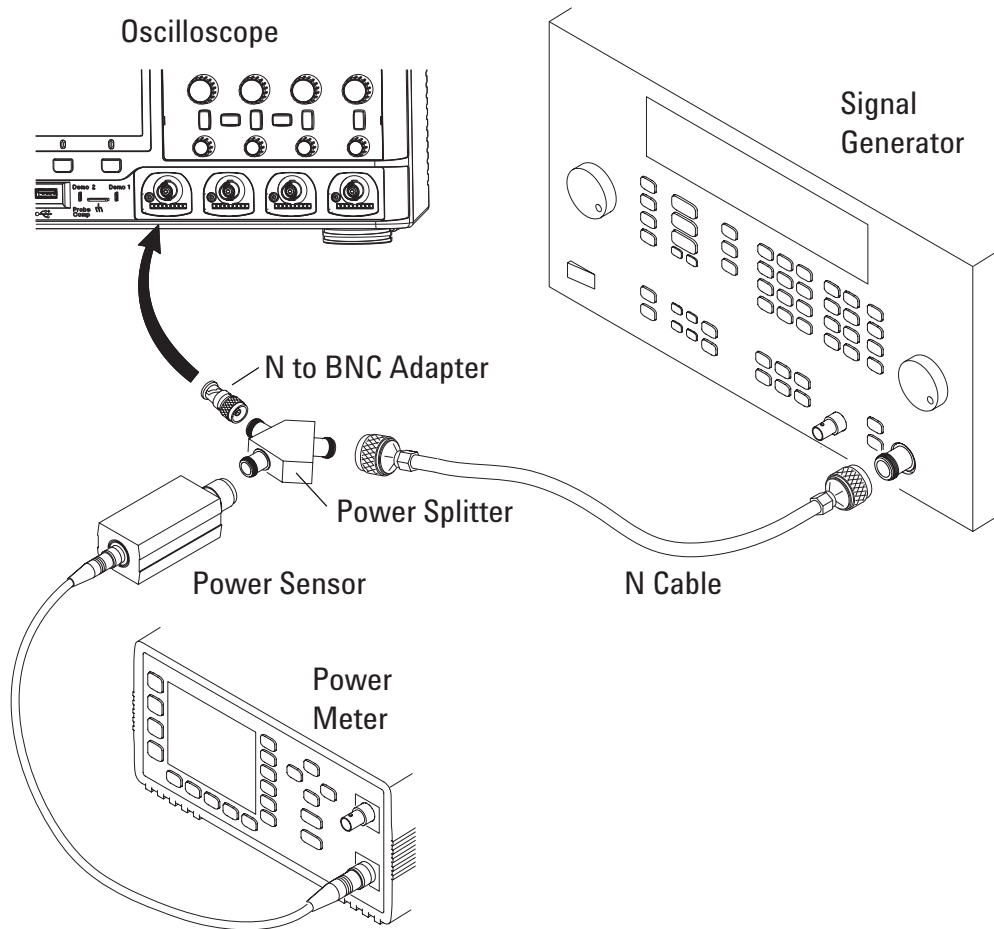

**Figure 7** Setting Up Equipment for Bandwidth (-3 dB) Verification Test

**2** Set up the power meter.

Set the power meter to display measurements in units of watts.

**3** Set up the oscilloscope.

- a** Press the **[Default Setup]** key.
- b** Set channel 1 **Coupling** to **DC**.

- c** With 2000 X-Series oscilloscopes, connect a 50 ohm feedthrough termination.  
  
With 3000 X-Series oscilloscopes, set channel 1 **Imped** to **50 Ohm**.
  - d** Set the time base to 500 ns/div.
  - e** Set the Volts/Div for channel 1 to 200 mV/div.
  - f** Press the [**Acquire**] key, then press the **Averaging** softkey.
  - g** Turn the Entry knob to set **# Avgs** to 8 averages.
- 4** Set the signal generator for 1 MHz and six divisions of amplitude.

The signal on the oscilloscope screen should be about five cycles at six divisions amplitude.

- 5** Set up the Amplitude measurement
- a** Press the [**Meas**] key.
  - b** Press the **Clear Meas** softkey and then the **Clear All** softkey.
  - c** Press the **Type:** softkey and use the Entry knob to select **AC RMS - Full Screen (Std Deviation)** within the select menu.
  - d** Press the **Add Measurement** softkey.
- 6** Note the oscilloscope AC RMS - FS(1) reading at the bottom of the screen. (This is the RMS value with any dc offset removed.)
- 7** Set the power meter Cal Factor % to the 1 MHz value on the calibration chart on the power sensor.
- 8** Note the reading on the power meter and covert to Vrms using the expression:

$$V_{in_{1MHz}} = \sqrt{P_{meas_{1MHz}} \times 50\Omega}$$

For example, if the power meter reading is 892 uW, then  $V_{in_{1MHz}} = (892 \times 10^{-6} * 50\Omega)^{1/2} = 211.2 \text{ mV}_{\text{rms}}$ .



- 9** Change the signal generator output frequency according to the maximum frequency for the oscilloscope using the following:
- 1 GHz Models: 1 GHz
  - 500 MHz Models: 500 MHz
  - 350 MHz Models: 350 MHz
  - 200 MHz Models: 200 MHz
  - 100 MHz Models: 100 MHz
  - 70 MHz Models: 70 MHz
- 10** Referencing the frequency from step 9, set the power meter Cal Factor % to the frequency value on the calibration chart on the power sensor.
- 11** Set the oscilloscope sweep speed according to the following:
- 1 GHz Models: 500 ps/div
  - 500 MHz Models: 1 ns/div
  - 350 MHz Models: 2 ns/div
  - 200 MHz Models: 2 ns/div
  - 100 MHz Models: 5 ns/div
  - 70 MHz Models: 5 ns/div
- 12** Note the oscilloscope Std Dev(1) reading at the bottom of the screen.
- 13** Note the reading on the power meter and convert to  $V_{rms}$  using the expression:

$$V_{in_{maxfreq}} = \sqrt{P_{meas_{maxfreq}} \times 50\Omega}$$

- 14** Calculate the response using the expression:

$$\text{response(dB)} = 20 \log_{10} \left[ \frac{V_{out_{maxfreq}} / V_{in_{maxfreq}}}{V_{out_{1MHz}} / V_{in_{1MHz}}} \right]$$

**Example** If:

$$P_{meas_{1MHz}} = 892 \text{ uW}$$

$$\text{Std Dev}(n)_{1MHz} = 210.4 \text{ mV}$$

## 2 Testing Performance

$$P_{\text{meas max\_freq}} = 687 \text{ uW}$$
$$\text{Std Dev}(n)_{\text{max freq}} = 161.6 \text{ mV}$$

Then after converting the values from the power meter to  $V_{\text{rms}}$ :

$$\text{response(dB)} = 20 \log_{10} \left[ \frac{161.6 \text{ mV} / 185.3 \text{ mV}}{210.4 \text{ mV} / 211.2 \text{ mV}} \right] = -1.16 \text{ dB}$$

- 15** The result from step 14 should be between +3.0 dB and -3.0 dB. Record the result in the Performance Test Record (see [page 63](#)).
- 16** Move the power splitter from the channel 1 to the channel 2 input.
- 17** Turn off the current channel and turn on the next channel using the channel keys.
- 18** Repeat steps 3 through 17 for the remaining channels, setting the parameters of the channel being tested where appropriate.

## To verify time base accuracy

This test verifies the accuracy of the time base. In this test you will measure the absolute error of the time base oscillator and compare the results to the specification.


**Table 15** Equipment Required to Verify Time Base Accuracy

Equipment	Critical Specifications	Recommended Model/Part
Signal Generator	100 kHz - 1 GHz, 0.01 Hz frequency resolution, jitter: < 2ps	Agilent N5181A
Cable	BNC, 3 feet	Agilent 10503A
50 Ohm Feedthrough Termination	50Ω BNC (f) to BNC (m), when testing 2000 X-Series oscilloscopes	Agilent 0960-0301

- 1 Set up the signal generator.
  - a Set the output to 10 MHz, approximately 1 V<sub>pp</sub> sine wave.
- 2 Connect the output of the signal generator to oscilloscope channel 1 using the BNC cable. When testing 2000 X-Series oscilloscopes, also connect a 50 ohm feedthrough termination between the channel 1 input and the BNC cable.
- 3 Set up the oscilloscope:
  - a Press [AutoScale].
  - b Set the oscilloscope Channel 1 vertical sensitivity to 200 mv/div.
  - c Set the oscilloscope horizontal sweep speed control to 5 ns/div.
  - d Adjust the intensity to get a sharp, clear trace.

## 2 Testing Performance

- e Adjust the oscilloscope's trigger level so that the rising edge of the waveform at the center of the screen is located where the center horizontal and vertical grid lines cross (center screen).
  - f Ensure the horizontal position control is set to 0.0 seconds.
- 4 Make the measurement.
- a Set oscilloscope horizontal sweep speed control to 1 ms/div.
  - b Set horizontal position control to +1 ms (rotate control CCW).
  - c Set the oscilloscope horizontal sweep speed control to 5 ns/div.
  - d Record the number of nanoseconds from where the rising edge crosses the center horizontal grid line to the center vertical grid line. The number of nanoseconds is equivalent to the time base error in ppm.
  - e Use the date code on the oscilloscope's serial tag to calculate the number of years since manufacture. Include any fractional portion of a year.

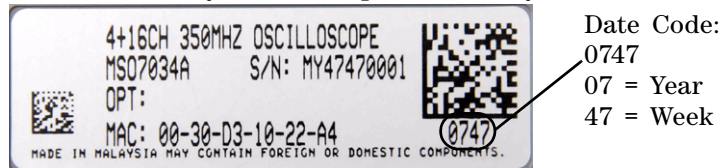

- f Use the following formula to calculate the test limits.  
Time base accuracy limit: 25 ppm  $\pm$ 5 ppm per year (aging)
- g Record the result and compare it to the limits in the Performance Test Record (see [page 63](#)).

## To verify trigger sensitivity

This test verifies the trigger sensitivity. In this test, you will apply a sine wave to the oscilloscope at the upper bandwidth limit. You will then decrease the amplitude of the signal to the specified levels, and check to see if the oscilloscope is still triggered.

Test limits for:


- Internal trigger sensitivity on all models:
  - < 10 mV/div: greater of 1 div or 5 mV<sub>pp</sub>
  - >= 10 mV/div: 0.6 div
- External trigger sensitivity on all models:
  - DC to 100 MHz: < 200 mV<sub>pp</sub>
  - 100 MHz - 200 MHz: < 350 mV<sub>pp</sub>

**Table 16** Equipment Required to Verify Trigger Sensitivity

Equipment	Critical Specifications	Recommended Model/Part
Signal Generator	25 MHz, 100 MHz, 350 MHz, 500 MHz, and 1 GHz sine waves	Agilent N5181A
Power splitter	Outputs differ < 0.15 dB	Agilent 11667A
Power Meter		Agilent N1914A
Power Sensor		Agilent E9304A or N8482A
Cable	BNC, Qty 3	Agilent 10503A
Adapter	N (m) to BNC (f), Qty 3	Agilent 1250-0780
Feedthrough	50Ω BNC (f) to BNC (m)	Agilent 0960-0301

## Test Internal Trigger Sensitivity (all models)

- 1 On the oscilloscope, press the **[Default Setup]** key.
- 2 Press the **[Mode/Coupling]** key; then, press the **Mode** softkey to select **Normal**.
- 3 Connect the equipment (see [Figure 8](#)).
  - a Connect the signal generator output to the oscilloscope channel 1 input.

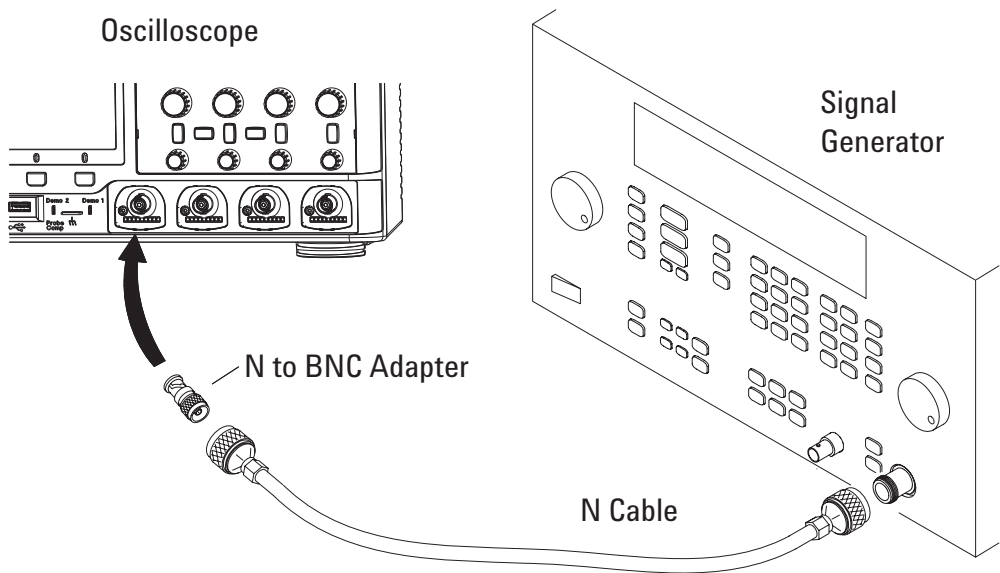

**Figure 8** Setting Up Equipment for Internal Trigger Sensitivity Test

- b With 2000 X-Series oscilloscopes, connect a 50 ohm feedthrough termination between the channel 1 input and the BNC cable.  
  
With 3000 X-Series oscilloscopes, set channel 1 **Imped** to **50 Ohm**.
- 4 To verify the trigger sensitivity at the oscilloscope's maximum bandwidth, set the output frequency of the

signal generator to the maximum bandwidth of the oscilloscope:

- 1 GHz models: 1 GHz.
- 500 MHz models: 500 MHz.
- 350 MHz models: 350 MHz.
- 200 MHz models: 200 MHz.
- 100 MHz models: 100 MHz.
- 70 MHz models: 70 MHz.

**5** Perform these steps to test at the 5 mV/div setting:

- a** Set the signal generator amplitude to about 10 mV<sub>pp</sub>.
- b** Press the [**AutoScale**] key.
- c** Set the time base to 10 ns/div.
- d** Set channel 1 to 5 mV/div.
- e** Decrease the amplitude from the signal generator until 1 vertical division of the signal (about 5 mV<sub>pp</sub>) is displayed.

The trigger is stable when the displayed waveform is stable. If the trigger is not stable, try adjusting the trigger level. If adjusting the trigger level makes the trigger stable, the test still passes. If adjusting the trigger does not help, see the “Troubleshooting” chapter. Then return here.

- f** Record the result as Pass or Fail in the Performance Test Record (see [page 63](#)).
- g** Repeat this step for the remaining oscilloscope channels.

**6** Perform these steps to test at the 10 mV/div setting:

- a** Set the signal generator amplitude to about 20 mV<sub>pp</sub>.
- b** Press the [**AutoScale**] key.
- c** Set the time base to 10 ns/div.
- d** Set channel 1 to 10 mV/div.
- e** Decrease the amplitude from the signal generator until 0.6 vertical divisions of the signal (about 6 mV<sub>pp</sub>) is displayed.

The trigger is stable when the displayed waveform is stable. If the trigger is not stable, try adjusting the trigger level. If adjusting the trigger level makes the trigger stable, the test still passes. If adjusting the trigger does not help, see the “Troubleshooting” chapter. Then return here.

- f** Record the result as Pass or Fail in the Performance Test Record (see [page 63](#)).
- g** Repeat this step for the remaining oscilloscope channels.


### Test External Trigger Sensitivity

This test applies to all models.

Verify the external trigger sensitivity at these settings:

- 100 MHz, 200 mV<sub>pp</sub>
  - 200 MHz, 350 mV<sub>pp</sub>
- 1** Connect the equipment (see [Figure 9](#)).
    - a** Use the N cable to connect the signal generator to the power splitter input.
    - b** Connect one output of the power splitter to the Aux Trig input through a 50Ω feedthrough termination.
    - c** Connect the power sensor to the other output of the power splitter.



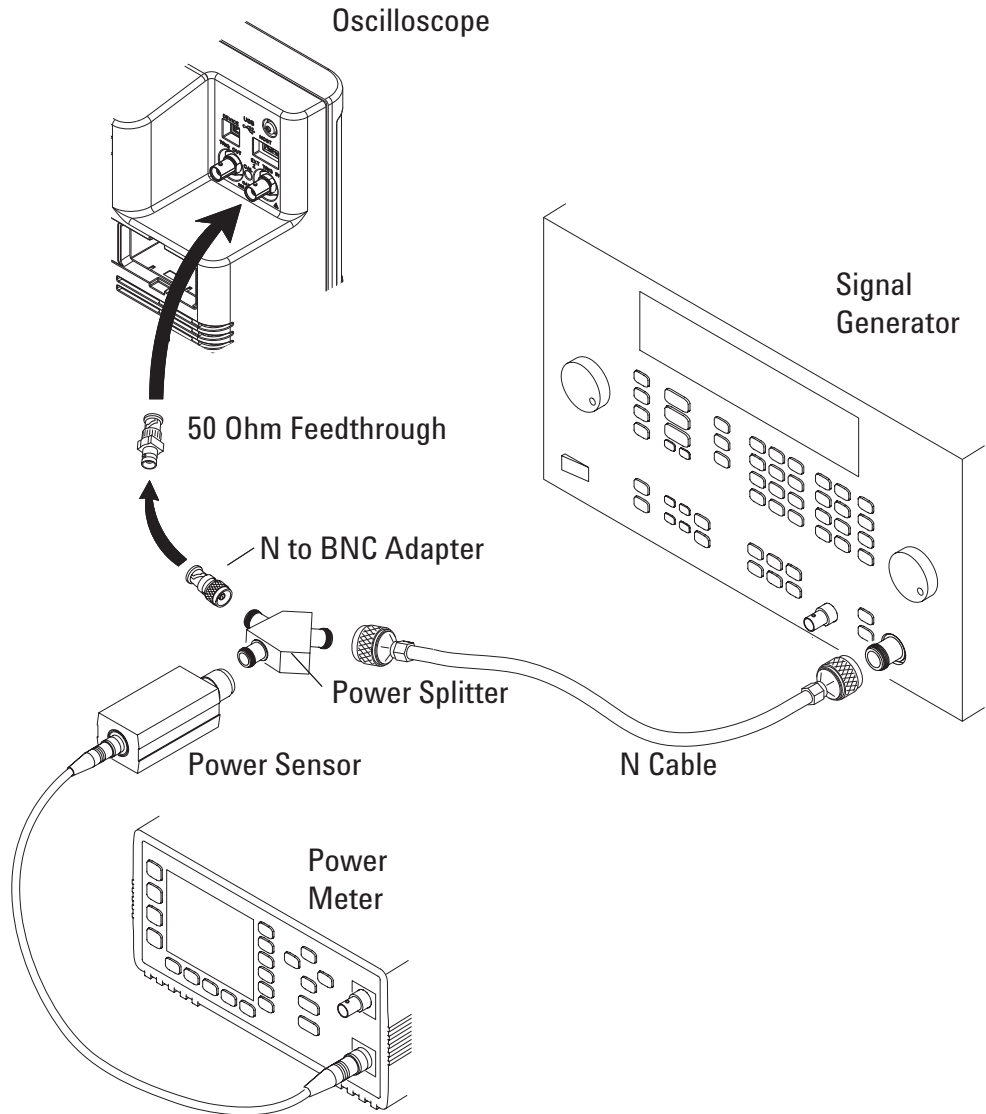

**Figure 9** Setting Up Equipment for 4-Channel External Trigger Sensitivity Test

- 2 Set up the oscilloscope.
  - a Press the [**Default Setup**] key.
  - b Press the [**Mode/Coupling**] key; then, press the **Mode** softkey to select **Normal**.
- 3 Change the signal generator output frequency to 100 MHz or 200 MHz.
- 4 Set the power meter Cal Factor % to the appropriate value (100 MHz or 200 MHz) on the calibration chart on the power sensor. If necessary, do a linear interpolation if a 100 MHz or 200 MHz factor is not included in the power meter’s calibration chart.
- 5 Adjust the signal generator output for reading on the power meter of:

Signal Generator Frequency	Calculation	Power Meter Reading
100 MHz	$200 \text{ mV}_{pp} = 70.71 \text{ mV rms,}$ $\text{Power} = V_{in}^2/50\Omega = 70.71 \text{ mV}^2/50\Omega$	100 $\mu\text{W}$
200 MHz	$350 \text{ mV}_{pp} = 123.74 \text{ mV rms,}$ $\text{Power} = V_{in}^2/50\Omega = 123.74 \text{ mV}^2/50\Omega$	306 $\mu\text{W}$

- 6 Press the [**Trigger**] key, then press the **Source** softkey to set the trigger source to **External**.
- 7 Check for stable triggering and adjust the trigger level if necessary. Triggering is indicated by the **Trig’d** indicator at the top of the display. When it is flashing, the oscilloscope is not triggered. When it is not flashing, the oscilloscope is triggered.
- 8 Record the results as Pass or Fail in the Performance Test Record (see [page 63](#)).

If the test fails, see the “Troubleshooting” chapter. Then return here.

# Agilent 2000 X-Series Oscilloscopes Performance Test Record

Serial No. _____		Test by _____	
Test Interval _____		Work Order No. _____	
Recommended Next Testing _____		Temperature _____	
<b>Threshold</b>	<b>Specification</b>	<b>Limits</b>	<b>Ch D7-D0</b>
<b>Accuracy Test</b>	5 V - 250 mV	4.750 V	_____
<b>(100 mV + 3% of threshold setting)</b>	5 V + 250 mV	5.250 V	_____
	-5 V - 250 mV	-5.250 V	_____
	-5 V + 250 mV	-4.750 V	_____
	0 V - 100 mV	-100 mV	_____
	0 V + 100 mV	100 mV	_____
<b>DC Vertical Gain Accuracy</b>			
<b>Range</b>	<b>Power Supply Setting</b>	<b>Test Limits</b>	<b>Channel 1 Channel 2 Channel 3* Channel 4*</b>
5 V/Div	35 V	33.8 V to 36.2 V	_____
2 V/Div	14 V	13.52 V to 14.48 V	_____
1 V/Div	7 V	6.76 V to 7.24 V	_____
500 mV/Div	3.5 V	3.38 V to 3.62 V	_____
200 mV/Div	1.4 V	1.352 V to 1.448 V	_____
100 mV/Div	700 mV	676 mV to 724 mV	_____
50 mV/Div	350 mV	338 mV to 362 mV	_____
20 mV/Div	140 mV	135.2 mV to 144.8 mV	_____
10 mV/Div	70 mV	67.6 mV to 72.4 mV	_____
5 mV/Div	35 mV	33.4 mV to 36.6 mV	_____
2 mV/Div	14 mV	12.72 mV to 15.28 mV	_____
1 mV/Div	7 mV	5.72 mV to 8.28 mV	_____

Continued on next page.

## 2 Testing Performance

<b>Dual Cursor Accuracy</b>				<b>Channel 1</b>	<b>Channel 2</b>	<b>Channel 3*</b>	<b>Channel 4*</b>
<b>Range</b>	<b>Power Supply Setting</b>	<b>Test Limits</b>					
5 V/Div	35 V	33.6 V to 36.4 V					
2 V/Div	14 V	13.44 V to 14.56 V					
1 V/Div	7 V	6.72 V to 7.28 V					
500 mV/Div	3.5 V	3.36 V to 3.64 V					
200 mV/Div	1.4 V	1.344 V to 1.456 V					
100 mV/Div	700 mV	672 mV to 728 mV					
50 mV/Div	350 mV	336 mV to 364 mV					
20 mV/Div	140 mV	134.4 mV to 145.6 mV					
10 mV/Div	70 mV	67.2 mV to 72.8 mV					
5 mV/Div	35 mV	33.2 mV to 36.8 mV					
2 mV/Div	14 mV	12.56 mV to 15.44 mV					
1 mV/Div	7 mV	5.56 mV to 8.44 mV					
<b>Bandwidth (-3 dB) Model</b>				<b>Channel 1</b>	<b>Channel 2</b>	<b>Channel 3*</b>	<b>Channel 4*</b>
	202x	-3 dB at 200 MHz					
	201x	-3 dB at 100 MHz					
	200x	-3 dB at 70 MHz					
<b>Time Base Accuracy Limits</b>				<b>Calculated time base accuracy limit (ppm)</b>	<b>Measured time base error (ppm)</b>	<b>Pass/Fail</b>	
Time Base Accuracy Limit: 25 ppm ±5 ppm per year (aging)							
<b>Internal Trigger Sensitivity</b>				<b>Channel 1</b>	<b>Channel 2</b>	<b>Channel 3*</b>	<b>Channel 4*</b>
	<b>Generator Setting</b>	<b>Test Limits</b>					
200 MHz models:	200 MHz	< 10 mV/div: greater of 1 div or 5 mVpp					
100 MHz models:	100 MHz						
70 MHz models:	70 MHz	>= 10 mV/div: 0.6 div					
<b>External Trigger Sensitivity</b>				<b>Ext Trig In</b>			
	<b>Generator Setting</b>	<b>Test Limits</b>					
	200 MHz	350 mV					
	100 MHz	200 mV					
* Where applicable							

# Agilent 3000 X-Series Oscilloscopes Performance Test Record

Serial No. _____ Test Interval _____ Recommended Next Testing _____	Test by _____ Work Order No. _____ Temperature _____				
<b>Threshold</b>	<b>Specification</b>	<b>Limits</b>	<b>Ch D7-D0</b>	<b>Ch D15-D8</b>	
<b>Accuracy Test</b>	5 V - 250 mV	4.750 V	_____	_____	
<b>(100 mV + 3% of threshold setting)</b>	5 V + 250 mV	5.250 V	_____	_____	
	-5 V - 250 mV	-5.250 V	_____	_____	
	-5 V + 250 mV	-4.750 V	_____	_____	
	0 V - 100 mV	-100 mV	_____	_____	
	0 V + 100 mV	100 mV	_____	_____	
<b>DC Vertical Gain Accuracy</b>					
<b>Range</b>	<b>Power Supply Setting</b>	<b>Test Limits</b>	<b>Channel 1</b>	<b>Channel 2</b>	<b>Channel 3*</b> <b>Channel 4*</b>
5 V/Div	35 V	34.2 V to 35.8 V	_____	_____	_____
2 V/Div	14 V	13.68 V to 14.32 V	_____	_____	_____
1 V/Div	7 V	6.84 V to 7.16 V	_____	_____	_____
500 mV/Div	3.5 V	3.42 V to 3.58 V	_____	_____	_____
200 mV/Div	1.4 V	1.368 V to 1.432 V	_____	_____	_____
100 mV/Div	700 mV	684 mV to 716 mV	_____	_____	_____
50 mV/Div	350 mV	342 mV to 358 mV	_____	_____	_____
20 mV/Div	140 mV	136.8 mV to 143.2 mV	_____	_____	_____
10 mV/Div	70 mV	68.4 mV to 71.6 mV	_____	_____	_____
5 mV/Div	35 mV	34.2 mV to 35.8 mV	_____	_____	_____
2 mV/Div	14 mV	13.36 mV to 14.64 mV	_____	_____	_____
1 mV/Div	7 mV	6.36 mV to 7.64 mV	_____	_____	_____

Continued on next page.

## 2 Testing Performance

<b>Dual Cursor Accuracy</b>							
<b>Range</b>	<b>Power Supply Setting</b>	<b>Test Limits</b>	<b>Channel 1</b>	<b>Channel 2</b>	<b>Channel 3*</b>	<b>Channel 4*</b>	
5 V/Div	35 V	34.0 V to 36.0 V	_____	_____	_____	_____	
2 V/Div	14 V	13.6 V to 14.4 V	_____	_____	_____	_____	
1 V/Div	7 V	6.8 V to 7.2 V	_____	_____	_____	_____	
500 mV/Div	3.5 V	3.4 V to 3.6 V	_____	_____	_____	_____	
200 mV/Div	1.4 V	1.36 V to 1.44 V	_____	_____	_____	_____	
100 mV/Div	700 mV	680 mV to 720 mV	_____	_____	_____	_____	
50 mV/Div	350 mV	340 mV to 360 mV	_____	_____	_____	_____	
20 mV/Div	140 mV	136 mV to 144 mV	_____	_____	_____	_____	
10 mV/Div	70 mV	68 mV to 72 mV	_____	_____	_____	_____	
5 mV/Div	35 mV	34 mV to 36 mV	_____	_____	_____	_____	
2 mV/Div	14 mV	13.2 mV to 14.8 mV	_____	_____	_____	_____	
1 mV/Div	7 mV	6.2 mV to 7.8 mV	_____	_____	_____	_____	
<b>Bandwidth (-3 dB)</b>				<b>Channel 1</b>	<b>Channel 2</b>	<b>Channel 3*</b>	<b>Channel 4*</b>
	<b>Model</b>	<b>Test Limits</b>					
	310x	-3 dB at 1 GHz	_____	_____	_____	_____	
	305x	-3 dB at 500 MHz	_____	_____	_____	_____	
	303x	-3 dB at 350 MHz	_____	_____	_____	_____	
	302x	-3 dB at 200 MHz	_____	_____	_____	_____	
	301x	-3 dB at 100 MHz	_____	_____	_____	_____	
<b>Time Base Accuracy Limits</b>				<b>Calculated time base accuracy limit (ppm)</b>	<b>Measured time base error (ppm)</b>	<b>Pass/Fail</b>	
Time Base Accuracy Limit: 25 ppm ±5 ppm per year (aging)				_____	_____	_____	
<b>Internal Trigger Sensitivity</b>				<b>Channel 1</b>	<b>Channel 2</b>	<b>Channel 3*</b>	<b>Channel 4*</b>
	<b>Generator Setting</b>	<b>Test Limits</b>					
1 GHz models:	1 GHz	< 10 mV/div: greater of 1 div or 5 mVpp	_____	_____	_____	_____	
500 MHz models:	350 MHz						
350 MHz models:	200 MHz	≥ 10 mV/div: 0.6 div	_____	_____	_____	_____	
200 MHz models:	100 MHz						
100 MHz models:							
<b>External Trigger Sensitivity</b>				<b>Ext Trig In</b>			
	<b>Generator Setting</b>	<b>Test Limits</b>					
	200 MHz	350 mV	_____				
	100 MHz	200 mV	_____				
* Where applicable							



## 3 Calibrating and Adjusting

This chapter explains how to adjust the oscilloscope for optimum operating performance. You should perform self-calibration according to the following recommendations:

- Every two years or after 4000 hours of operation
- If the ambient temperature is  $>10$  °C from the calibration temperature
- If you want to maximize the measurement accuracy

The amount of use, environmental conditions, and experience with other instruments help determine if you need shorter adjustment intervals.

### Let the Equipment Warm Up Before Adjusting

Before you start the adjustments, let the oscilloscope and test equipment warm up for at least 30 minutes.

### Read All Cautions and Warnings

Read the following cautions and warning before making adjustments or performing self-calibration.

#### **WARNING**

#### **HAZARDOUS VOLTAGES!**

Read the safety notice at the front of this book before proceeding. Maintenance is performed with power supplied to the oscilloscope and with the protective covers removed. Only trained service personnel who are aware of the hazards involved should perform the maintenance. Whenever possible, perform the procedures with the power cord removed from the oscilloscope.



#### CAUTION

##### **REMOVE POWER TO AVOID DAMAGE!**

Do not disconnect any cables or remove any assemblies with power applied to the oscilloscope. Otherwise, damage to the oscilloscope can occur.

---

#### CAUTION

##### **USE EXTERNAL FAN TO REDUCE TEMPERATURE!**

When you must operate the oscilloscope with its cover and main shield removed, use an external fan to provide continuous air flow over the samplers (the ICs with heat sinks on them). Air flow over the samplers is reduced when the cover and main shield is removed, which leads to higher than normal operating temperatures. Have the fan blow air across the system board where the heat sinks are located. If the cover is removed but the main shield remains installed and the bottom holes are not blocked, the instrument will cool properly.

---

#### CAUTION

##### **AVOID DAMAGE TO ELECTRONIC COMPONENTS!**

Electrostatic discharge (ESD) can damage electronic components. When you use any of the procedures in this chapter, use proper ESD precautions. As a minimum, place the oscilloscope on a properly grounded ESD mat and wear a properly grounded ESD strap.

---



## User Calibration

Perform user-calibration:

- Every two years or after 4000 hours of operation.
- If the ambient temperature is  $>10^{\circ}$  C from the calibration temperature.
- If you want to maximize the measurement accuracy.

The amount of use, environmental conditions, and experience with other instruments help determine if you need shorter User Cal intervals.

User Cal performs an internal self-alignment routine to optimize the signal path in the oscilloscope. The routine uses internally generated signals to optimize circuits that affect channel sensitivity, offset, and trigger parameters. Disconnect all inputs and allow the oscilloscope to warm up before performing this procedure.

Performing User Cal will invalidate your Certificate of Calibration. If NIST (National Institute of Standards and Technology) traceability is required perform the procedures in [Chapter 2](#) in this book using traceable sources.

### To perform User Cal


- 1 Disconnect all inputs from the front and rear panels, including the digital channels cable on an MSO, and allow the oscilloscope to warm up before performing this procedure.
- 2 Press the rear-panel CAL button to disable calibration protection..
- 3 Connect short (12 inch maximum) equal length cables to each analog channel's BNC connector on the front of the oscilloscope. You will need two equal-length cables for a

### 3 Calibrating and Adjusting

2-channel oscilloscope or four equal-length cables for a 4-channel oscilloscope.

Use 50 $\Omega$  RG58AU or equivalent BNC cables when performing User Cal.


- a For a 2-channel oscilloscope, connect a BNC tee to the equal length cables. Then connect a BNC(f)-to-BNC(f) (also called a barrel connector) to the tee as shown below.

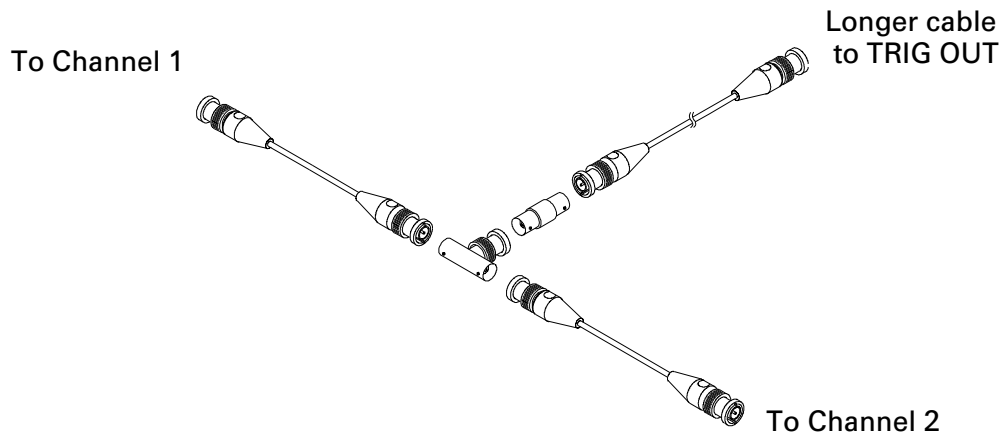

**Figure 10** User Calibration cable for 2-channel oscilloscope

- b For a 4-channel oscilloscope, connect BNC tees to the equal-length cables as shown below. Then connect a

BNC(f)-to-BNC(f) (barrel connector) to the tee as shown below.

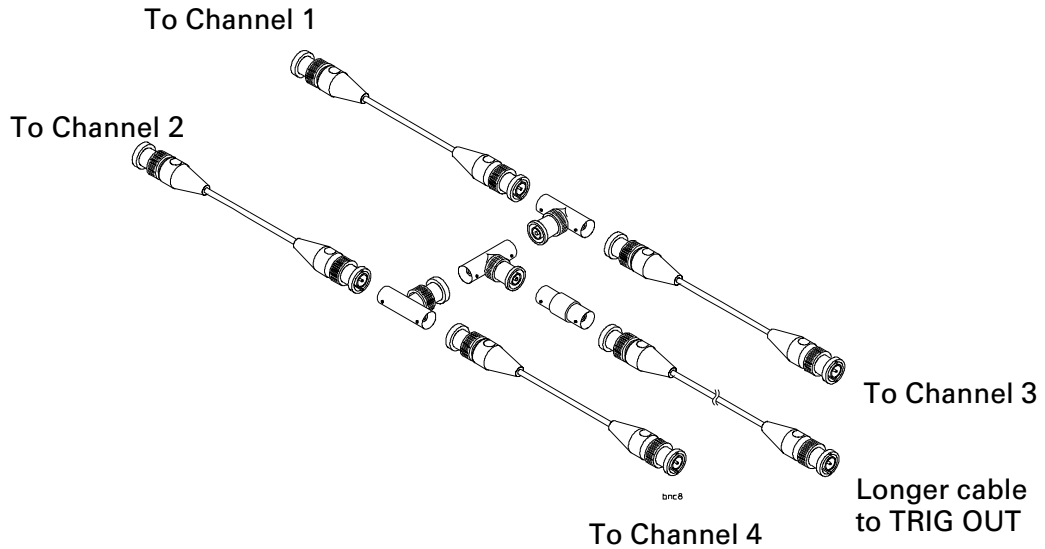

**Figure 11** User Calibration cable for 4-channel oscilloscope

- 4** Connect a BNC cable (40 inches maximum) from the TRIG OUT connector on the rear panel to the BNC barrel connector.
- 5** Press the **[Utility]** key; then, press the **Service** softkey.
- 6** Begin the Self Cal by pressing the **Start User Cal** softkey.

## User Cal Status

Pressing the **User Cal Status** softkey displays the following summary results of the previous User Cal, and the status of probe calibrations for probes that can be calibrated. Note that AutoProbes do not need to be calibrated, but InfiniiMax probes can be calibrated.

Results:

User Cal date:

Change in temperature since last User Cal:

Failure:

Comments:

Probe Cal Status:



## 4 Troubleshooting

Solving General Problems with the Oscilloscope 74

Verifying Basic Operation 77

Troubleshooting Internal Assemblies 83

### **Read All Cautions and Warnings**

Before you begin any troubleshooting, read all Warning and Cautions in the “Troubleshooting” section.

This chapter begins with “Solving General Problems with the Oscilloscope”. It tells you what to do in these cases:

- If there is no display.
- If there is no trace display.
- If the trace display is unusual or unexpected.
- If you cannot see a channel.

Next, this chapter describes procedures for “Verifying Basic Operation” of the oscilloscope:

- To power-on the oscilloscope.
- To perform hardware self test.
- To perform front panel self test.
- To verify default setup.
- To perform an Auto Scale on the Probe Comp signal.
- To compensate passive probes.

Finally, this chapter describes procedures for “Troubleshooting Internal Assemblies” when performing



assembly-level repair for 350 MHz, 500 MHz, and 1 GHz bandwidth oscilloscopes:

- To prepare for internal assembly troubleshooting.
- To check the system board power supply test points.
- To check the interboard supply connector voltages.
- To check the line filter board AC output.
- To check the power switch.
- To check the power supply DC output.
- To check the display supplies.
- To check the keyboard supplies.
- To check the fan.

## Solving General Problems with the Oscilloscope

This section describes how to solve general problems that you may encounter while using the Agilent 2000/3000 X-Series oscilloscopes.

After troubleshooting the oscilloscope, if you need to replace parts, refer to [Chapter 6](#), “Replaceable Parts,” starting on page 145.

### If there is no display

- ✓ Check that the power cord is firmly seated in the oscilloscope power receptacle.
- ✓ Check that the power source is live.
- ✓ Check that the front-panel power switch is on.

- ✓ If there is still no display, go to the troubleshooting procedures in this chapter.

## If there is no trace display

- ✓ Check that the Intensity (on the front panel) is adjusted correctly.
- ✓ Recall the default setup by pressing **[Default Setup]**. This will ensure that the trigger mode is Auto.
- ✓ Check that the probe clips are securely connected to points in the circuit under test, and that the ground is connected.
- ✓ Check that the circuit under test is powered on.
- ✓ Press the **[AutoScale]** key.
- ✓ Obtain service from Agilent Technologies, if necessary.

## If the trace display is unusual or unexpected

- ✓ Check that the Horizontal time/division setting is correct for the expected frequency range of the input signals.
- ✓ The sampling speed of the oscilloscope depends on the time/division setting. It may be that when time/division is set to slower speeds, the oscilloscope is sampling too slowly to capture all of the transitions on the waveform. Use peak detect mode.
- ✓ Check that all oscilloscope probes are connected to the correct signals in the circuit under test.
- ✓ Ensure that the probe's ground lead is securely connected to a ground point in the circuit under test. For high-speed measurements, each probe's individual ground lead should also be connected to a ground point closest to the signal point in the circuit under test.

- ✓ Check that the trigger setup is correct.
- ✓ A correct trigger setup is the most important factor in helping you capture the data you desire. See the *User's Guide* for information about triggering.
- ✓ Check that persistence in the Display menu is turned off, then press the **Clear Display** softkey.
- ✓ Press the [**Auto Scale**] key.

### If you cannot see a channel

- ✓ Recall the default setup by pressing [**Default Setup**]. This will ensure that the trigger mode is Auto.
- ✓ Check that the oscilloscope probe's BNC connector is securely attached to the oscilloscope's input connector.
- ✓ Check that the probe clips are securely connected to points in the circuit under test.
- ✓ Check that the circuit under test is powered on.

You may have pressed the [**Auto Scale**] key before an input signal was available.

Performing the checks listed here ensures that the signals from the circuit under test will be seen by the oscilloscope. Perform the remaining checks in this topic to make sure the oscilloscope channels are on, and to obtain an automatic setup.

- ✓ Check that the desired oscilloscope channels are turned on.
  - a** Press the analog channel key until it is illuminated.
  - b** On models with the MSO option, press the digital channels [**Digital**] key until it is illuminated.
- ✓ Press the [**Auto Scale**] key to automatically set up all channels.



## Verifying Basic Operation

### To power-on the oscilloscope

- 1 Connect the power cord to the rear of the oscilloscope, then to a suitable ac voltage source.

The oscilloscope power supply automatically adjusts for input line voltages in the range of 100 to 240 VAC. Ensure that you have the correct line cord (see [page 145](#)). The power cord provided is matched to the country of origin.

**WARNING****AVOID INJURY.**

Always operate the oscilloscope with an approved three conductor power cable. Do not negate the protective action of the three conductor power cable.

---

- Press the power switch.
    - When the oscilloscope is turned on, the front panel LEDs will briefly light up in groups from bottom to top.
    - Next the Agilent logo appears on the display.
    - Next a message will appear with tips on getting started using the oscilloscope. At this time you can press any key to remove the message and view the display. Or you can wait and the message will automatically disappear.
    - It will take a total of about 20-30 seconds for the oscilloscope to go through its basic self test and power-up routine.
- 2 Proceed to “[To perform hardware self test](#)” on page 78.

## To perform hardware self test

Pressing [**Utility**] > **Service** > **Hardware Self Test** performs a series of internal procedures to verify that the oscilloscope is operating properly.

It is recommended you run Hardware Self Test:

- After experiencing abnormal operation.
- For additional information to better describe an oscilloscope failure.
- To verify proper operation after the oscilloscope has been repaired.

Successfully passing Hardware Self Test does not guarantee 100% of the oscilloscope's functionality. Hardware Self Test is designed to provide an 80% confidence level that the oscilloscope is operating properly.

## To perform front panel self test

Pressing [**Utility**] > **Service** > **Front Panel Self Test** lets you test the front panel keys and knobs as well as the oscilloscope display.

Follow the on-screen instructions.

Failures in the front panel self test indicate problems with the keyboard, keypad, or display.

## To verify default setup

The oscilloscope is designed to turn on with the setup from the last turn on or previous setup.


To recall the default setup:

- 1 Press the [**Default Setup**] key.

This returns the oscilloscope to its default settings and places the oscilloscope in a known operating condition. The major default settings are:

- **Horizontal:**
  - main mode.
  - 100 us/div scale.
  - 0 s delay.
  - center time reference.
- **Vertical:**
  - Channel 1 on.
  - 5 V/div scale.
  - dc coupling.
  - 0 V position.
  - probe factor to 1.0 if an AutoProbe probe is not connected to the channel.
- **Trigger:**
  - Edge trigger.
  - Auto sweep mode.
  - 0 V level.
  - channel 1 source.
  - dc coupling.
  - rising edge slope.
  - 40 ns holdoff time.
- **Display:**
  - 20% grid intensity.
  - persistence off.

- **Other:**
  - Acquire mode normal.
  - Run/Stop to Run.
  - cursor measurements off.

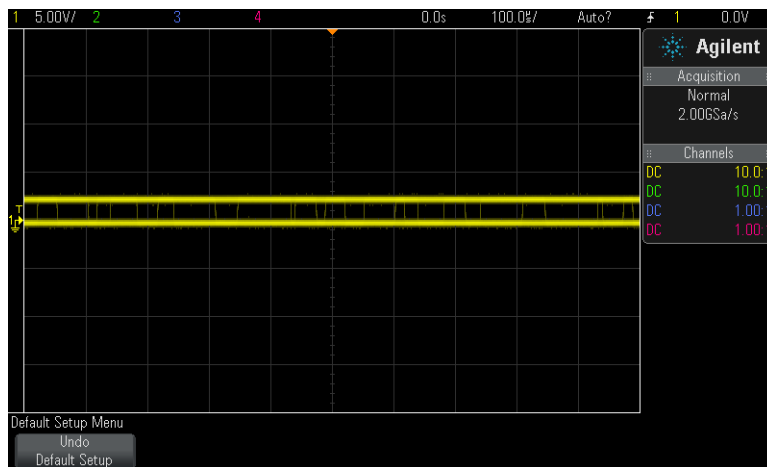


**Figure 12** Default setup screen

- 2 If your screen looks substantially different, replace the system board.

### To perform an Auto Scale on the Probe Comp signal

- 1 Press the [**Default Setup**] key. The oscilloscope is now configured to its default settings.
- 2 Connect an oscilloscope probe from channel 1 to the **Probe Comp** signal terminal on the front panel.
- 3 Connect the probe's ground lead to the ground terminal that is next to the **Demo 2** (Probe Comp) terminal.
- 4 Press [**AutoScale**].

- 5 You should see a waveform on the oscilloscope's display similar to this:

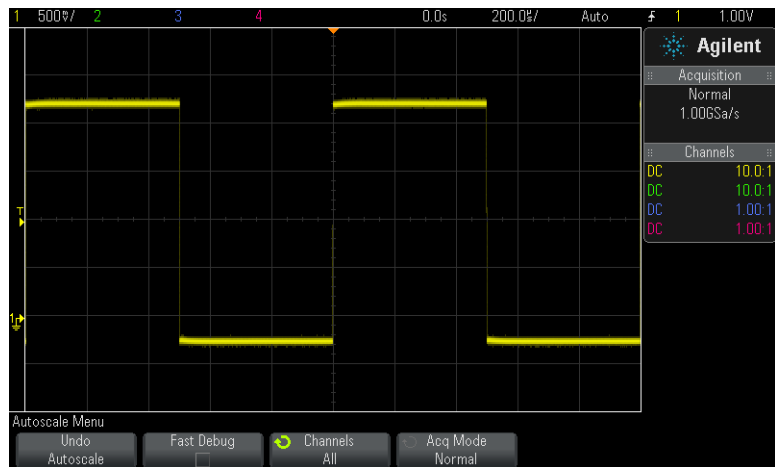

If you see the waveform, but the square wave is not shaped correctly as shown above, perform the procedure [“To compensate passive probes”](#) on page 81.

If you do not see the waveform, ensure your power source is adequate, the oscilloscope is properly powered-on, and the probe is connected securely to the front-panel analog channel input BNC and to the Demo 2 (Probe Comp) terminal.

- 6 If you still do not see the waveform, use the troubleshooting flowchart in this chapter to isolate the problem.

## To compensate passive probes


You should compensate your passive probes to match their characteristics to the oscilloscope's channels. A poorly compensated probe can introduce measurement errors.

- 1 Perform the procedure “To perform an Auto Scale on the Probe Comp signal” on page 80
- 2 Press the channel key to which the probe is connected ([1], [2], etc.).
- 3 In the Channel Menu, press **Probe**.
- 4 In the Channel Probe Menu, press **Probe Check**; then, follow the instructions on-screen.

If necessary, use a nonmetallic tool (supplied with the probe) to adjust the trimmer capacitor on the probe for the flattest pulse possible.

On the N2862/63/90 probes, the trimmer capacitor is the yellow adjustment on the probe tip. On other probes, the trimmer capacitor is located on the probe BNC connector.

**Perfectly compensated**



**Over compensated**



**Under compensated**



comp.cdr

**Figure 13** Example pulses

- 5 Connect probes to all other oscilloscope channels (channel 2 of a 2-channel oscilloscope, or channels 2, 3, and 4 of a 4-channel oscilloscope).
- 6 Repeat the procedure for each channel.

The process of compensating the probes serves as a basic test to verify that the oscilloscope is functional.

## Troubleshooting Internal Assemblies

The service policy for 200 MHz and lower bandwidth oscilloscopes is unit replacement, so there is no internal assembly troubleshooting for these models.

The service policy for 350 MHz, 500 MHz, and 1 GHz bandwidth oscilloscopes is assembly level replacement. You can use the procedures described in this section to help identify assemblies that need replacement.

Generally, you want to make sure cables to the assembly are good and properly seated. Then, you check that the assembly is supplied with the proper power. If cables are good and the power is good, but the assembly still does not function properly, it must be replaced.

If you need parts or assistance from Agilent Technologies to repair your instrument, go to [www.agilent.com](http://www.agilent.com) and locate the service facility for your area.

### Equipment Required for Troubleshooting Internal Assemblies

The equipment listed in this table is required to troubleshoot the oscilloscope.

**Table 17** Equipment Required to Troubleshoot the Oscilloscope

Equipment	Critical Specifications	Recommended Model/Part
Digital multimeter	Accuracy $\pm 0.05\%$ 1 mV resolution	Agilent 34401A
Oscilloscope	Capable of measuring $\geq 500$ MHz signal. 1 M $\Omega$ input impedance.	Agilent DS06102A, MS06102A, DS07104A/B, or MS07104A/B

## To prepare for internal assembly troubleshooting

### WARNING

#### HAZARDOUS VOLTAGES EXIST — REMOVE POWER FIRST !

The procedures described in this section are performed with power supplied to the oscilloscope and with the protective covers removed. Only trained service personnel who are aware of the hazards involved should perform the procedures. Whenever possible, perform the procedures with the power cord removed from the oscilloscope. Read the safety notice at the back of this book before proceeding.

---

### WARNING



#### HAZARDOUS VOLTAGES EXIST — HIGH VOLTAGE IS PRESENT ON POWER SUPPLY HEAT SINKS !

The power supply heat sinks of the 2000/3000 X-Series oscilloscopes are at a high potential. This presents an electric shock hazard. Protect yourself from electric shock by keeping this area covered or by not coming in contact with the heat sinks when the power cord is attached to the oscilloscope!

---

### CAUTION

#### REMOVE POWER TO AVOID DAMAGE !

Do not disconnect any cables or remove any assemblies while power is applied to the oscilloscope, or damage to the oscilloscope can occur.

---

### CAUTION

#### AVOID ESD DAMAGE TO COMPONENTS !


ELECTROSTATIC DISCHARGE (ESD) can damage electronic components. Use proper ESD precautions when doing any of the procedures in this chapter. As a minimum, place the oscilloscope on a properly grounded ESD mat and wear a properly grounded ESD strap.

---

- 1 Disconnect any external cables from the front panel.
- 2 Disconnect the power cord.
- 3 Remove the bucket assembly following the instructions on [page 105](#).
- 4 Remove the power supply shield following the instructions on [page 107](#).
- 5 Separate the front and rear decks following the instructions on [page 110](#).



- 6 Re-connect the interboard supply cable as shown in the following figure.

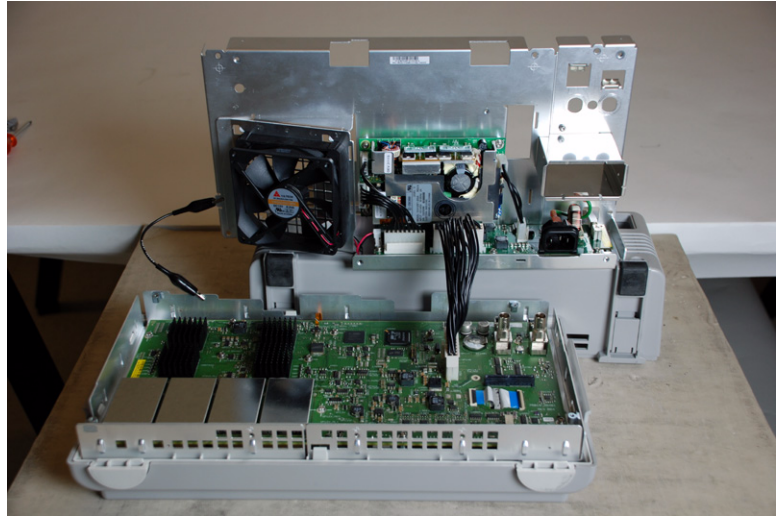

**Figure 14** Setup for troubleshooting internal assemblies

### CAUTION

#### **MAKE SURE EARTH GROUND IS MAINTAINED FOR THE FRONT DECK !**

For example, connect a cable with alligator clips between the rear deck chassis and the front deck chassis, or connect a BNC cable from one of the BNCs on the system board to a known grounded BNC on your workbench.

Other advice:

- Place the front deck in a cover or rest it on a cloth to prevent scuffing the front panel knobs.
  - Because of the short length of the interboard supply cable, elevate the rear deck to prevent strain on the cable.
- 7 Make sure the keyboard cable, display cable, display backlight power cable, and all other cables are properly connected.

### CAUTION

#### **USE AN EXTERNAL FAN TO AVOID OVERHEATING COMPONENTS !**


When you remove the oscilloscope cover and main shield, use an external fan to provide continuous air flow over the heat sinks. Air flow over the heat sinks is reduced when the cover and main shield are removed, which leads to higher than normal operating temperatures. Have the fan blow air across the system board where the heat sinks are located. Otherwise, damage to the components can occur.

If the cover of a 2000/3000 X-Series oscilloscope is removed but the main shield remains installed and the bottom holes are not blocked, the instrument will cool properly.

---

## Flowchart for Troubleshooting Internal Assemblies

The following flowchart is a simplified overview of troubleshooting the oscilloscope's internal assemblies.

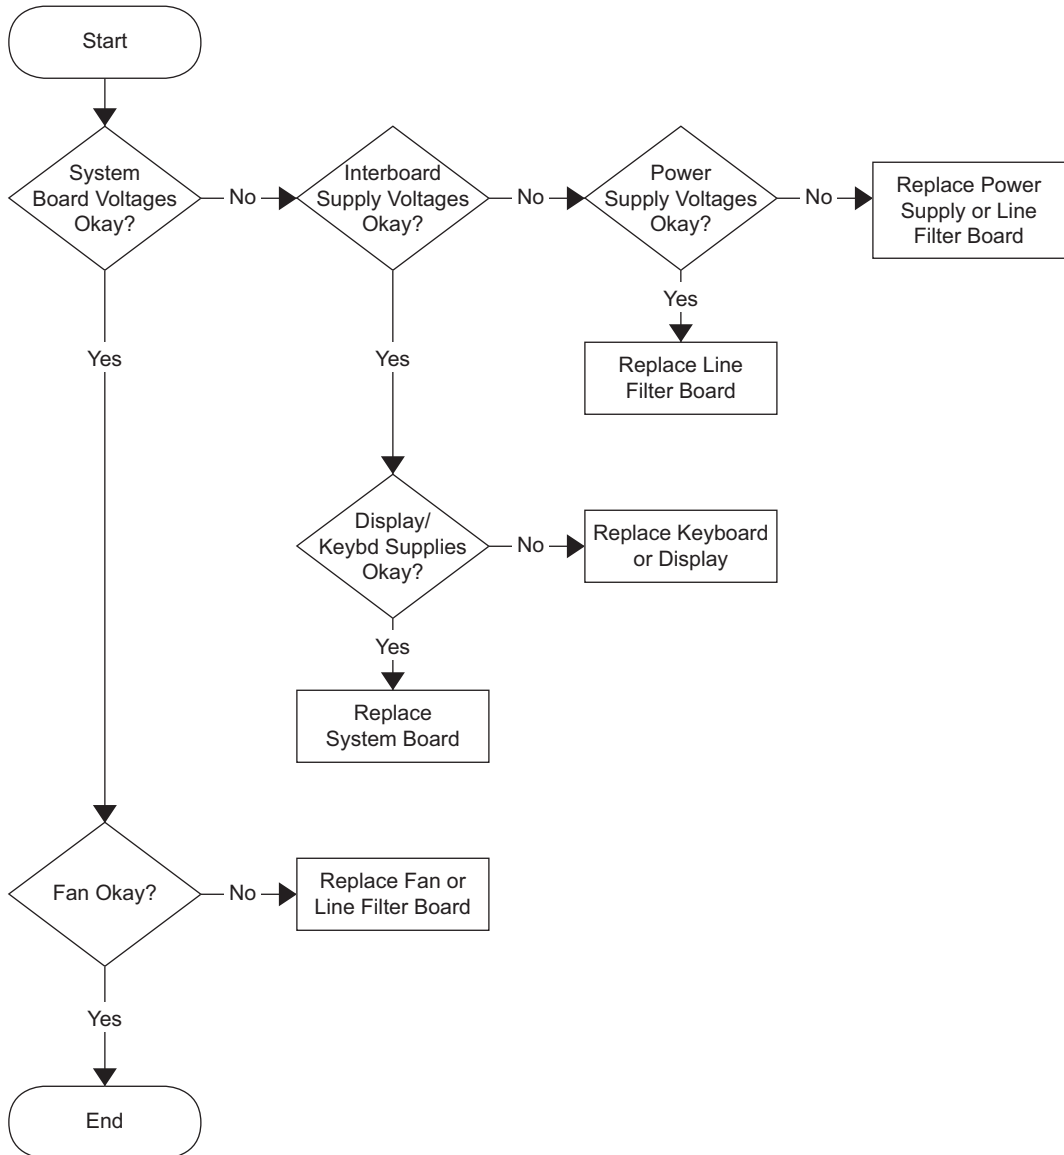

## System Board Drawings

Use these drawings to locate test points on the 350 MHz, 500 MHz, and 1 GHz bandwidth oscilloscopes' system board.

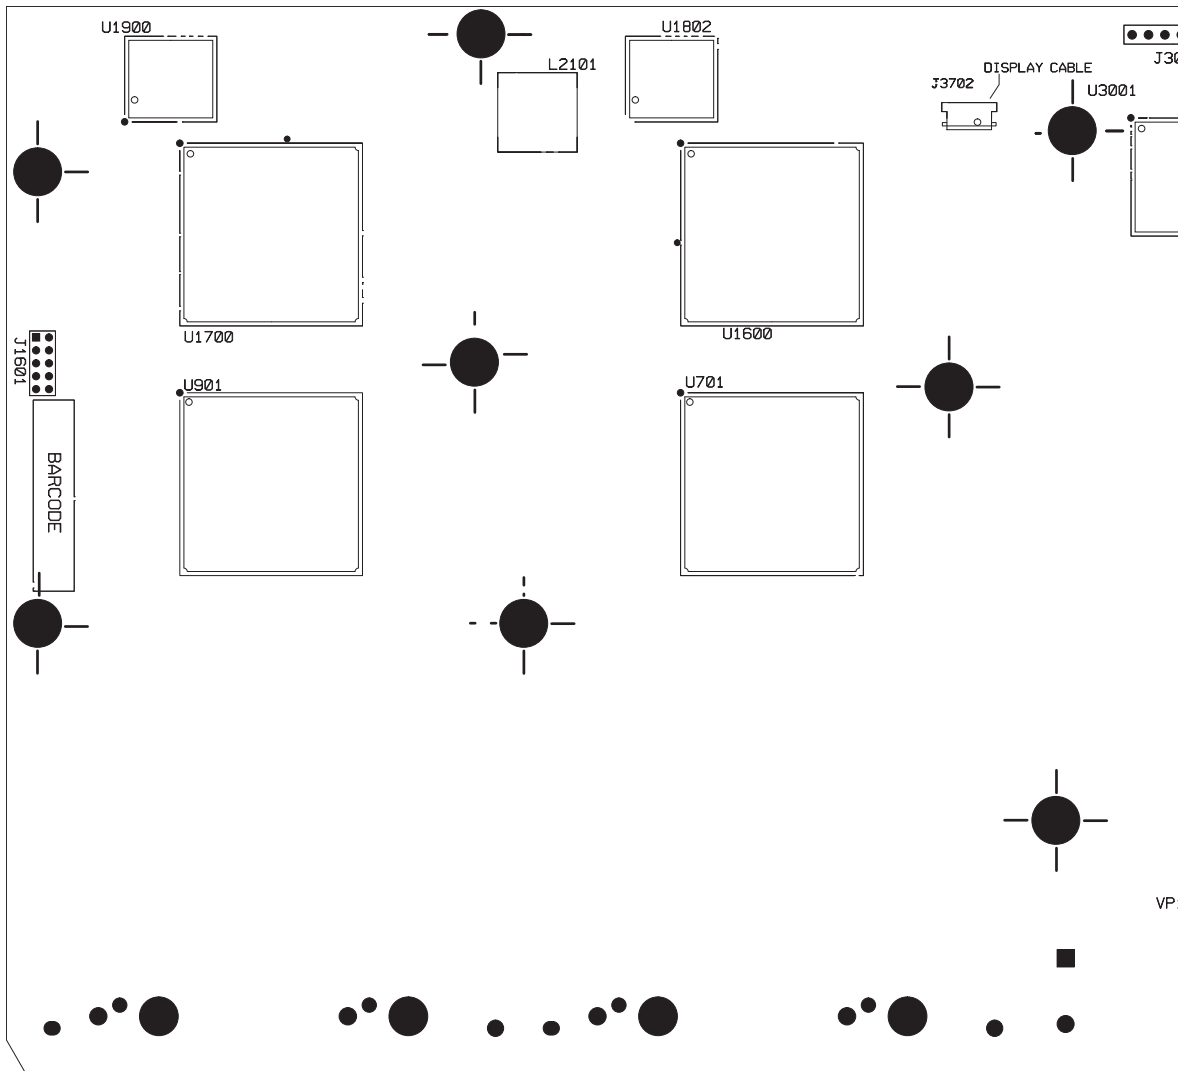


Figure 15 System Board Test Points/Connectors - Top Side, Left

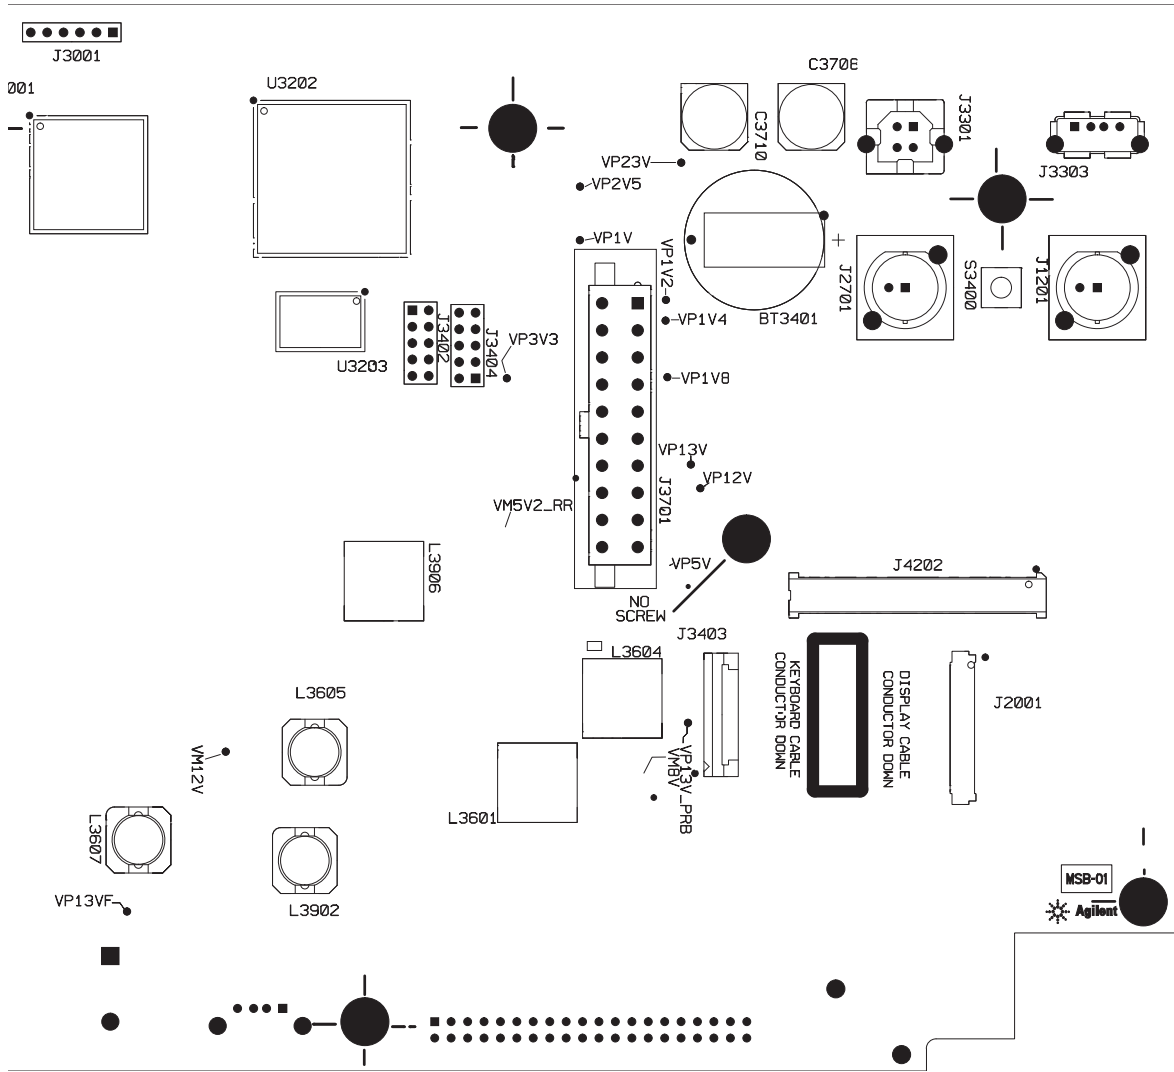


Figure 16 System Board Test Points/Connectors - Top Side, Right

## To check the system board power supply test points

This procedure checks the power supply test points on the system board (see See [Figure 16](#) on page 89). Values outside the expected range help identify bad assemblies.

- 1 Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2 Connect the negative lead of the multimeter to a ground point on the oscilloscope.
- 3 Connect the power cord, and turn on the oscilloscope.
- 4 First check the bulk power supply voltage:

Test Point (near J3701)	Expected Value	Assemblies Supplied	If Good	If Bad
VP13V	+13 V $\pm$ 3%	All	Indicates power supply is good.	Go to <a href="#">“To check the interboard supply connector voltages”</a> on page 91 and check VP13V there.

- 5 Next, check the supplies coming from the line filter board:

Test Point (near J3701)	Expected Value	Assemblies Supplied	If Good	If Bad
VP5V	+5 V $\pm$ 3%	Keyboard, System Board	Indicates supply coming from line filter board is good.	Go to <a href="#">“To check the interboard supply connector voltages”</a> on page 91.
VP12V	+12 V $\pm$ 3%	System Board		
VP1V8	+1.8 V $\pm$ 3%	System Board		
VP1V4	+1.4 V $\pm$ 3%	System Board		
VP1V	+1 V $\pm$ 3%	System Board		
VP1V2	+1.2 V $\pm$ 3%	System Board		
VP2V5	+2.5 V $\pm$ 3%	System Board		
VP3V3	+3.3 V $\pm$ 3%	LCD, System Board		

6 Finally, check the supplies coming from the system board:

Test Point (near J3701)	Expected Value	Assemblies Supplied	If Good	If Bad
VM12V	-11.5 V to -12.5 V	System Board	Indicates supply coming from system board is good.	Replace the system board.
VM8V	-7.814 V to -8.333 V	System Board		Replace the system board.
VM5V2	-5.023 V to -5.329 V	System Board		Replace the system board.
VP13VF	+13 V $\pm$ 3%	System Board		Replace the system board.
VP23V	+22.84 V to +24.2 V	Display Backlight Power		Go to <a href="#">“To check the display supplies”</a> on page 97.
VP13V_PRB	+13 V $\pm$ 3%	AutoProbe Interface		Go to <a href="#">“To check the keyboard supplies”</a> on page 98.

## To check the interboard supply connector voltages

This procedure checks the voltages on the line filter board’s interboard supply connector (J108) when the interboard supply cable is disconnected.

If these voltages are bad when the cable is connected but good when the cable is disconnected, it indicates problems with the system board, keyboard, or display assemblies that are being supplied.

- 1 Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2 Connect the negative lead of the multimeter to a ground point on the oscilloscope.
- 3 With the power cord disconnected, disconnect the interboard supply cable from the system board and the line filter board.
- 4 Connect the power cord, and turn on the oscilloscope.

- 5 Check the voltages on the line filter board's interboard supply connector J108.

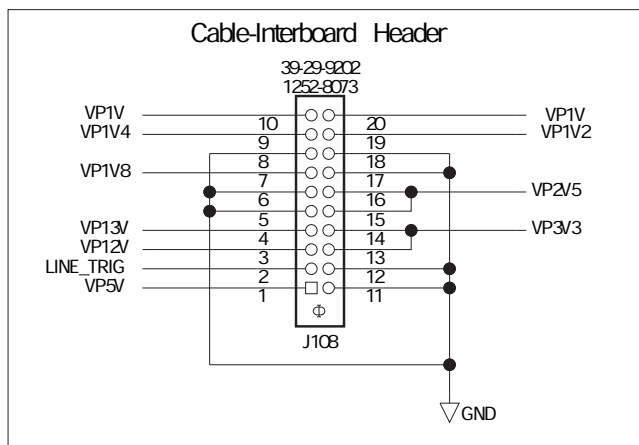


Figure 17 Line filter board interboard supply connector J108

- a If the VP13V bulk supply was bad at the system board test point, check it again at the interboard supply connector J108:

Test Point (near J3701)	Expected Value	Assemblies Supplied	If Good	If Bad
VP13V	+13 V $\pm$ 3%	Whole system	<p>If good when the interboard supply cable is disconnected from the system board, but bad when the interboard supply cable is connected, this indicates a problem with either the cable or the assemblies supplied,</p> <ol style="list-style-type: none"> <li>1 First, test the interboard supply cable for opens or shorts using the DMM.</li> <li>2 If the interboard supply cable is good, replace the system board.</li> </ol>	Go to <a href="#">“To check the line filter board AC output”</a> on page 93 to test whether the AC input to the power supply is good.




- b If the VP13V bulk supply was good at the system board test point, but other supplies coming from the line filter board were bad at the system board test points, check them again at the interboard supply connector J108:

Test Point (near J3701)	Expected Value	Assemblies Supplied	If Good	If Bad
VP5V	+5 V $\pm$ 3%	Keyboard, System Board	Go to <a href="#">“To check the keyboard supplies”</a> on page 98.	Replace the line filter board.
VP12V	+12 V $\pm$ 3%	System Board	If good when the interboard supply cable is disconnected from the system board, but bad when the interboard supply cable is connected, this indicates a problem with either the cable or the assemblies supplied, <b>1</b> First, test the interboard supply cable for opens or shorts using the DMM. <b>2</b> If the interboard supply cable is good, replace the system board.	Replace the line filter board.
VP1V8	+1.8 V $\pm$ 3%	System Board		Replace the line filter board.
VP1V4	+1.4 V $\pm$ 3%	System Board		Replace the line filter board.
VP1V	+1 V $\pm$ 3%	System Board		Replace the line filter board.
VP1V2	+1.2 V $\pm$ 3%	System Board		Replace the line filter board.
VP2V5	+2.5 V $\pm$ 3%	System Board		Replace the line filter board.
VP3V3	+3.3 V $\pm$ 3%	LCD, System Board	Go to <a href="#">“To check the display supplies”</a> on page 97.	Replace the line filter board.

## To check the line filter board AC output

When the 13 V bulk power is not being properly supplied, this procedure tests the AC input to the power supply to determine whether there is a problem with the line filter board.

- 1** Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2** Connect the power cord, and turn on the oscilloscope.
- 3** Verify that AC power is present at J1 on the power supply using a DVM and probes as shown in the following picture (remember this is an AC voltage measurement!).

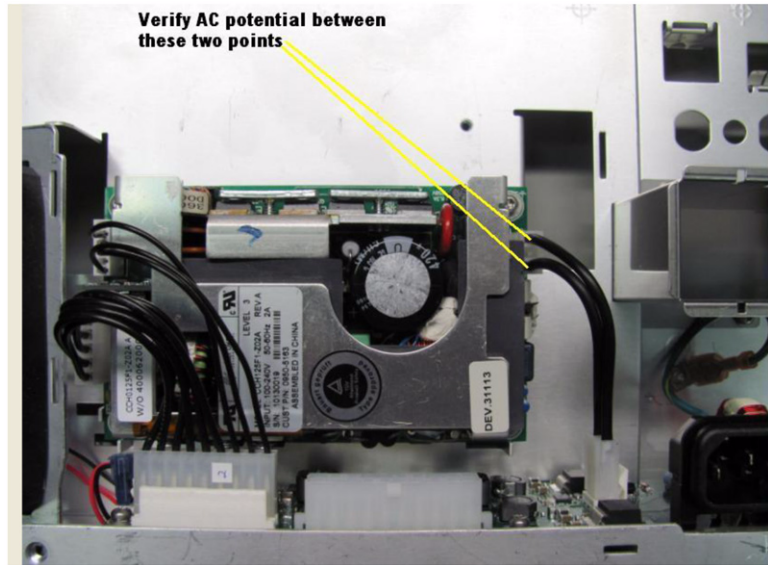


**Figure 18** Verify line filter board AC output

- If you have AC power equal to what is being applied to J100 (power cord socket) on the line filter assembly, the AC mains portion of the line filter assembly is probably okay.
- If there is no AC power at J1 of the power supply, there is something wrong with the AC mains section of the line filter assembly, and you need to *replace the line filter assembly*.
- If there is AC power at J1 of the power supply, but the instrument still will not power ON when the power switch (S100) is in the ON position, go to [“To check the power switch”](#) on page 95.

## To check the power switch

This procedure verifies the operation of the power switch (S100) on the line filter board assembly.

- 1 Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2 With the power cord disconnected, verify the operation of the power switch (S100) using a DMM in the resistance measurement mode and a set of probes.
  - a Connect the “-” side of the DMM to pin 6 of J107 on the line filter board and the “+” side of the DMM to pin 6 of J6 on the power supply.

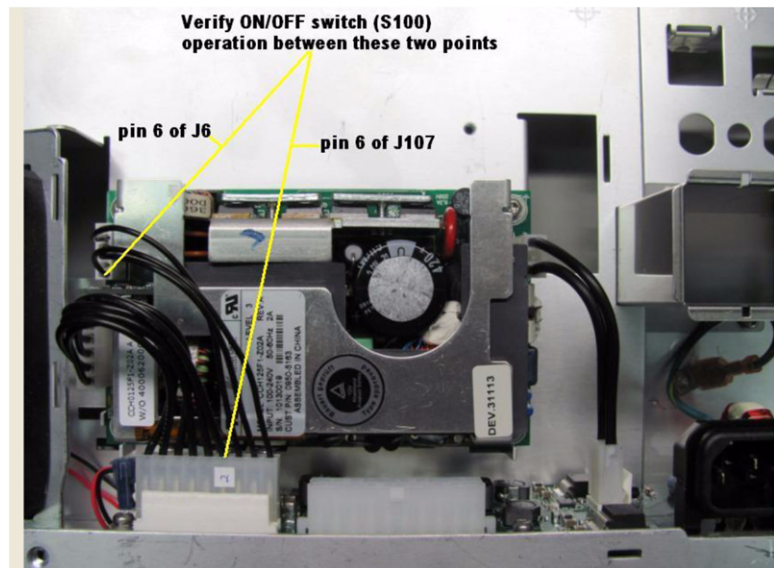

**Figure 19** Verify power switch operation

- With S100 in the OFF position (switch contacts closed) you should measure less than 1 ohm of resistance.
- With S100 in the ON position (switch contacts open) you should measure at least 8k ohms.

If you do not measure these two values:

- There may be something wrong with the power switch (S100 on the line filter assembly).
- The cable that connects between J107 on the line filter assembly and J6 and J4 on the power supply could be wired wrong.
- The power supply could be defective.

To figure out which of these is causing the problem, see [“To check the power supply DC output”](#) on page 96.

### To check the power supply DC output

This procedure checks the power supply DC output after verifying the AC input is good and checking the power switch operation.

- 1 Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2 Connect the negative lead of the multimeter to a ground point on the oscilloscope.
- 3 With the power cord disconnected:
  - a Disconnect the DC supply cable that is plugged into J107 of the line filter assembly.
- 4 Connect the power cord, and turn on the oscilloscope.
- 5 Verify there is +13V between pins 1 (+) and 4 (-) of J4 on the power supply.

If +13V is not present between pins 1 and 4 of J4 on the power supply, *replace the power supply.*

If +13V is present between pins 1 and 4 of J4 on the power supply, either the cable is wired incorrectly or the power switch S100 is defective or has a solder short to ground between one or some of its pins.

- a Turn off the oscilloscope, and disconnect the power cord.
- b Replace the DC supply cable.
- c Connect the power cord, and turn on the oscilloscope.
- d Check again to see if the output of the power supply turns ON and OFF as you actuate the power switch S100.

If replacing the cable does not fix the problem, there is something wrong with the power switch S100, and you must *replace the line filter assembly*.

## To check the display supplies

This procedure checks the display supply voltages on the system board test points when the display backlight power cable and the display cable are disconnected.

If one or both of these voltages are bad when the cables are connected but good when the cables are disconnected, it indicates problems with the display assembly.

- 1 Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2 Connect the negative lead of the multimeter to a ground point on the oscilloscope.
- 3 With the power cord disconnected:
  - a Disconnect the display backlight power cable from the system board connector J3702.
  - b Disconnect the display cable from the system board connector J2001.
- 4 Connect the power cord, and turn on the oscilloscope.

5 Check the display supplies:

Test Point (near J3701)	Expected Value	Assemblies Supplied	If Good	If Bad
VP23V	+22.84 V to +24.2 V	Display Backlight Power	Replace the display assembly.	Replace the system board.
VP3V3	+3.3 V $\pm$ 3%	LCD, System Board	If good when the display cable is disconnected from the system board, but bad when the display cable is connected, this indicates a problem with either the display cable or the display assembly, <ol style="list-style-type: none"> <li>1 Turn off the oscilloscope, and disconnect the power cord.</li> <li>2 Replace the display cable.</li> <li>3 Connect the power cord, and turn on the oscilloscope.</li> </ol> If the problem is not fixed, replace the display assembly.	Replace the line filter board.

## To check the keyboard supplies

This procedure checks the keyboard supply voltages on the system board test points when the keyboard cable is disconnected.

If one or both of these voltages are bad when the keyboard cable is connected but good when the cable is disconnected, it indicates problems with the keyboard assembly.

- 1 Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2 Connect the negative lead of the multimeter to a ground point on the oscilloscope.

- 3 With the power cord disconnected:
  - a Disconnect the keyboard cable from the system board connector J3403.
- 4 Connect the power cord, and turn on the oscilloscope.
- 5 Check the keyboard supplies:

Test Point (near J3701)	Expected Value	Assemblies Supplied	If Good	If Bad
VP5V	+5 V $\pm$ 3%	Keyboard, System Board	If good when the keyboard cable is disconnected from the system board, but bad when the keyboard cable is connected, this indicates a problem with either the keyboard cable or the keyboard.	Replace the line filter board.
VP13V_PRB	+13 V $\pm$ 3%	AutoProbe Interface	<ol style="list-style-type: none"> <li>1 Turn off the oscilloscope, and disconnect the power cord.</li> <li>2 Replace the keyboard cable.</li> <li>3 Connect the power cord, and turn on the oscilloscope.</li> <li>a If the problem is not fixed, replace the keyboard.</li> </ol>	Replace the system board.

## To check the fan

The fan speed is controlled by a circuit on the line filter board.

If the fan is running, perform the hardware self-tests. Go to [“To perform hardware self test”](#) on page 78.

If the fan is not running, it may be defective. Follow these steps:

- 1 Follow the instructions in [“To prepare for internal assembly troubleshooting”](#) on page 84.
- 2 Disconnect the fan cable from the line filter board.
- 3 Connect the power cord, and turn on the oscilloscope.


## 4 Troubleshooting

- 4 Measure the fan voltage at the connector on the line filter board.

See the following figure for the location of the fan connector.


- 5 If the fan voltage is approximately +6.5 Vdc at room temperature, replace the fan. If the fan voltage is not approximately +6.5 Vdc, *replace the line filter board*.

The proper voltage range depending on temperature is between +6.5 Vdc to +8.5 Vdc.

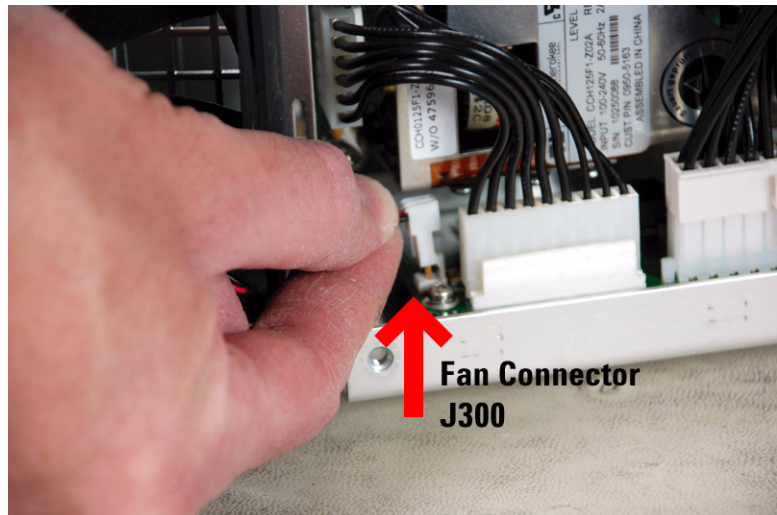

**Figure 20** Location of the Fan Connector



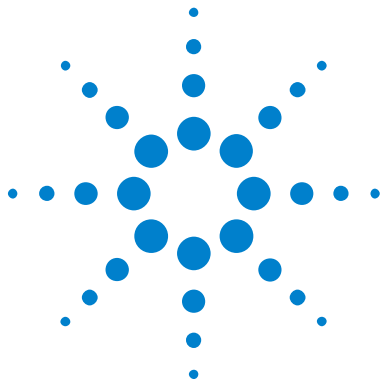

## 5 Replacing Assemblies

The service policy for 200 MHz and lower bandwidth oscilloscopes is unit replacement, so the instructions in this chapter are primarily for the 350 MHz, 500 MHz, and 1 GHz bandwidth oscilloscopes.

This chapter describes how to remove assemblies from an oscilloscope. To install a replacement assembly after you have removed an old one, follow the instructions in reverse order.

The parts shown in the following figures are representative and may look different from what you have in your oscilloscope.

### **Instructions for removable assemblies include:**

- To remove the front panel knobs [104](#)
- To remove the bucket assembly [105](#)
- To remove the power supply [136](#)
- To remove the rear deck assembly [110](#)
- To remove the acquisition board [117](#)
- To remove the front panel assembly [122](#)
- To remove the display assembly [129](#)
- To remove the fan assembly [134](#)
- To remove the power supply [136](#)
- To remove the line filter board [139](#)



### Tools Used for Disassembly

Use these tools to remove and replace the oscilloscope assemblies:

- T6, T10, and T20 TORX drivers.
- 5/8-inch socket driver or adjustable wrench (for BNC nuts).
- Flat head screw driver.

### See how the Oscilloscope Parts Fit Together

An exploded view of the oscilloscope is included in the “Replaceable Parts” chapter. It shows the individual part numbers used in the assemblies, and shows you how the parts fit together.

### Read All Warnings and Cautions

Read the following warnings and cautions before removing and replacing any assemblies in the oscilloscope.

#### WARNING

##### HAZARDOUS VOLTAGES!

Read the safety summary at the back of this book before proceeding. Maintenance is performed with power supplied to the oscilloscope and with the protective covers removed. Only trained service personnel who are aware of the hazards involved should perform the maintenance. Whenever possible, perform the procedures with the power cord removed from the oscilloscope.

---

#### WARNING



##### AVOID ELECTRICAL SHOCK!

Hazardous voltages exist on the LCD assembly and power supply. To avoid electrical shock:

- 1 Disconnect the power cord from the oscilloscope.
- 2 Wait at least three minutes for the capacitors in the oscilloscope to discharge before you begin disassembly.

Read the Safety Summary at the back of this manual before you begin.

---

**CAUTION****REMOVE POWER TO AVOID DAMAGE!**

Remove power before you begin to remove and replace assemblies. Do not remove or replace assemblies while the oscilloscope is turned on, or damage to the components can occur.

---

**CAUTION****AVOID DAMAGE TO ELECTRONIC COMPONENTS!**

ELECTROSTATIC DISCHARGE (ESD) can damage electronic components. When doing any of the procedures in this chapter, use proper ESD precautions. As a minimum, you should place the instrument on a properly grounded ESD mat and wear a properly grounded ESD strap.

---

## To remove the front panel knobs

The front panel knobs must be removed prior to localized front panel overlay installation or front panel disassembly.

- 1 Gently pull on the front panel knobs to remove them.




**Figure 21** Removing the front panel knobs

## To remove the bucket assembly

Removing the bucket assembly gives you access to the rear deck, fan assembly, power supply cover, power supply assembly, and power switch assembly.

- 1 Using T20 TORX driver, remove the four screws securing the bucket assembly to rear deck assembly.

You must open the storage compartment lid to access one of the screws.

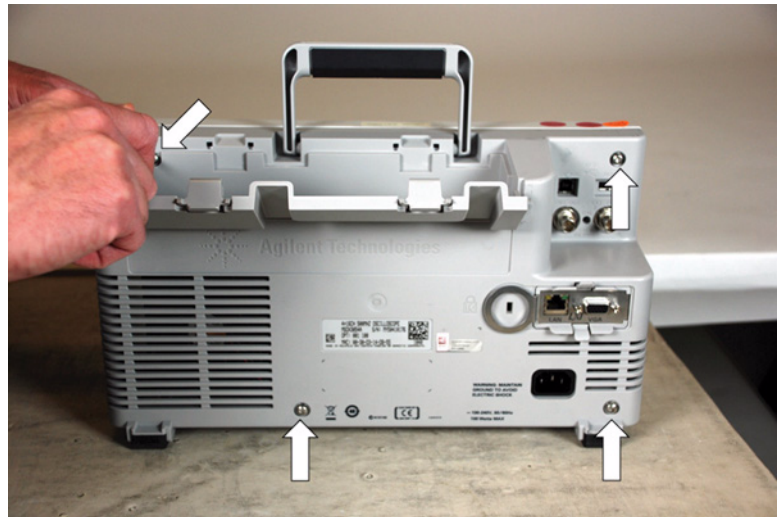

**Figure 22** Removing the bucket screws

## 5 Replacing Assemblies


- 2 Carefully slide bucket assembly back away from rear deck assembly.



**Figure 23** Removing bucket assembly

## To remove the power supply shield

- 1 Using a TORX T10 driver, locate and remove the screw securing the power supply shield to the rear deck.

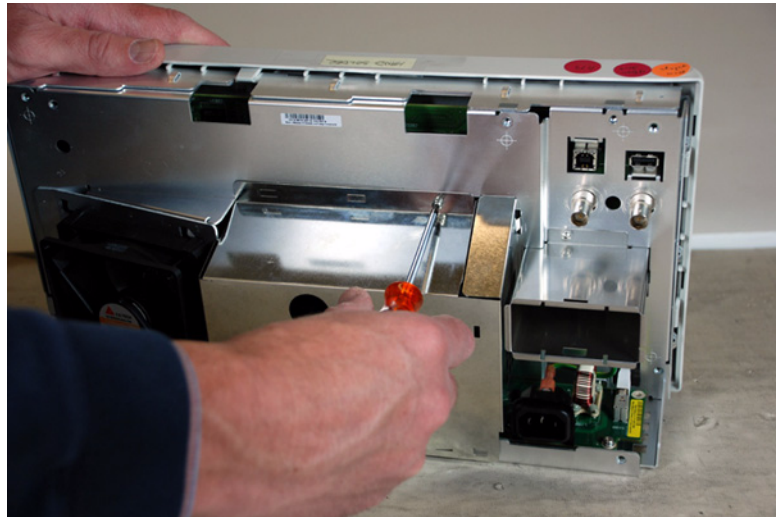

**Figure 24** Removing the power supply shield screw

**WARNING**

Sheet metal parts may have sharp edges. Handle with care to avoid injury.

---

## 5 Replacing Assemblies

- 2 When the screw has been removed, unclip the right side of the shield from the rear deck.




**Figure 25** Unclipping the power supply shield right side

- 3 When the screw has been removed and the shield has been unclipped, carefully remove the shield by lifting the



cover upward and then pulling its tabs out of the slots on the rear deck.

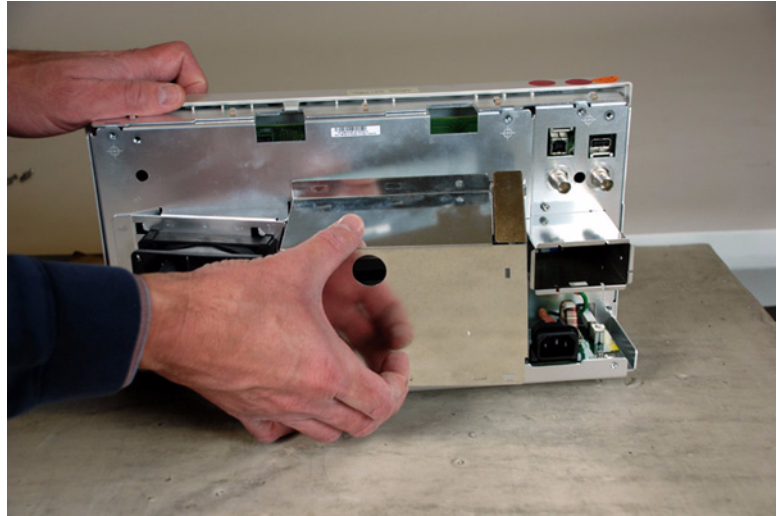

**Figure 26** Removing the power supply shield - lift and pull out

## To remove the rear deck assembly


Removing the rear deck allows access to the front deck and acquisition board.

- 1 Remove BNC securing nuts and washers.



**Figure 27** Removing the BNC nuts and washers


- 2 Using a T10 TORX driver, locate and remove all screws securing rear deck to front deck.

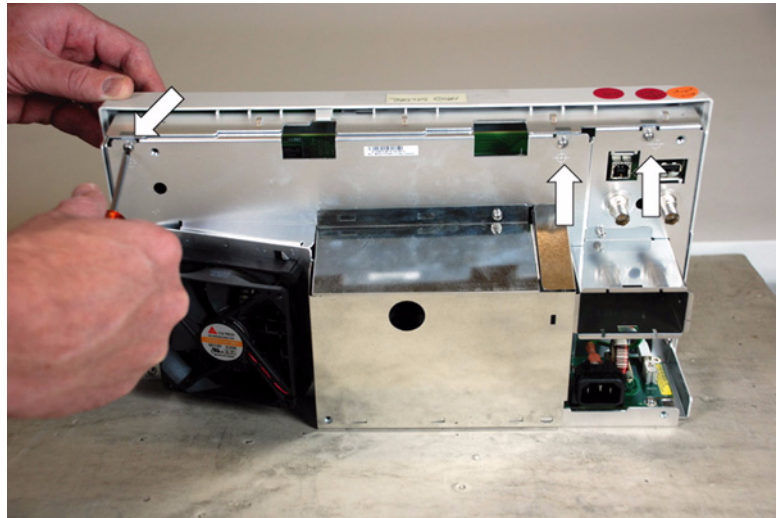


**Figure 28** Removing the top rear deck screws



**Figure 29** Removing the bottom right rear deck screw

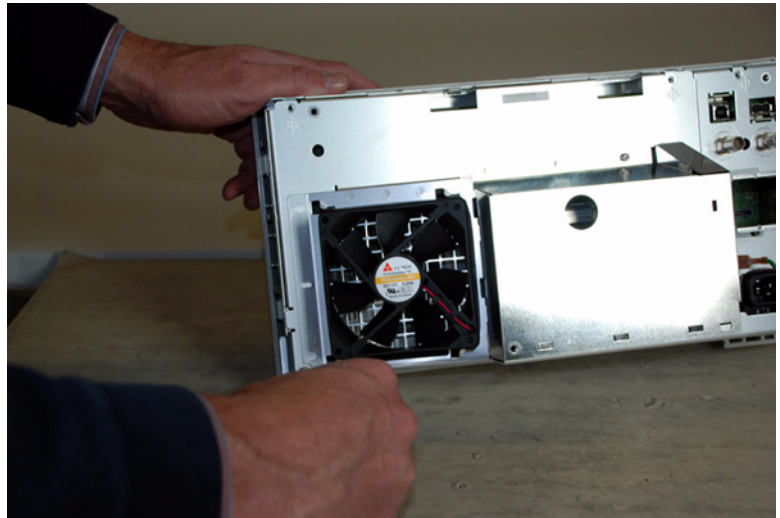

**Figure 30** Removing the bottom left rear deck screw

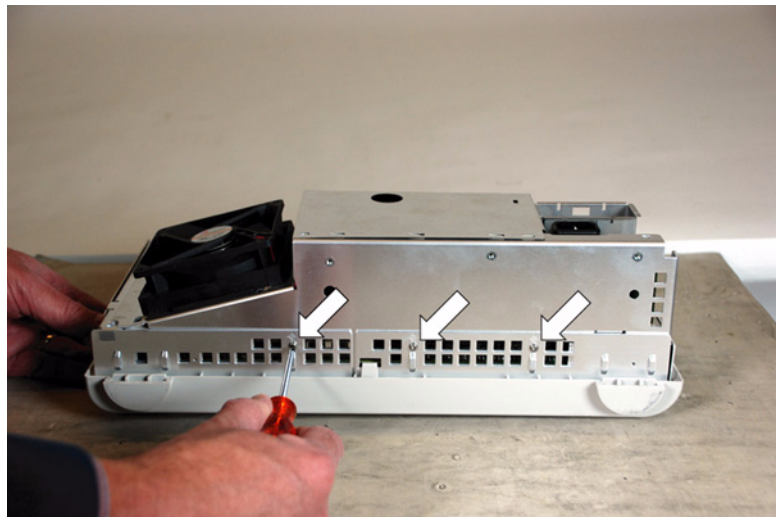

**Figure 31** Removing the bottom rear deck screws




**Figure 32** Removing the option module guide to acquisition board screw

- 3** If the power supply shield has not already been removed, do that now. See [“To remove the power supply shield”](#) on page 107.

## 5 Replacing Assemblies


- 4 Disconnect the interboard supply cable from the acquisition board.

You may need to use a screwdriver to pry the connector latch.

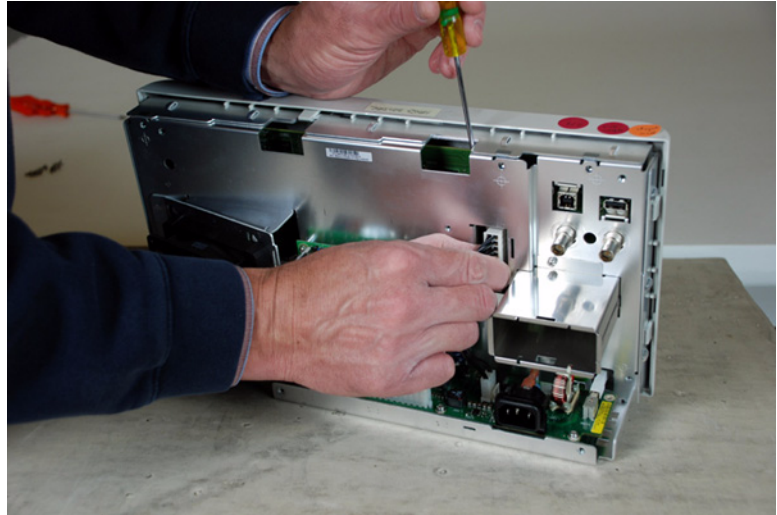

**Figure 33** Disconnecting the interboard supply cable from the acquisition board


- 5 Carefully separate the rear deck from the front deck.
  - a Lift the front bezel latch that holds the rear deck.

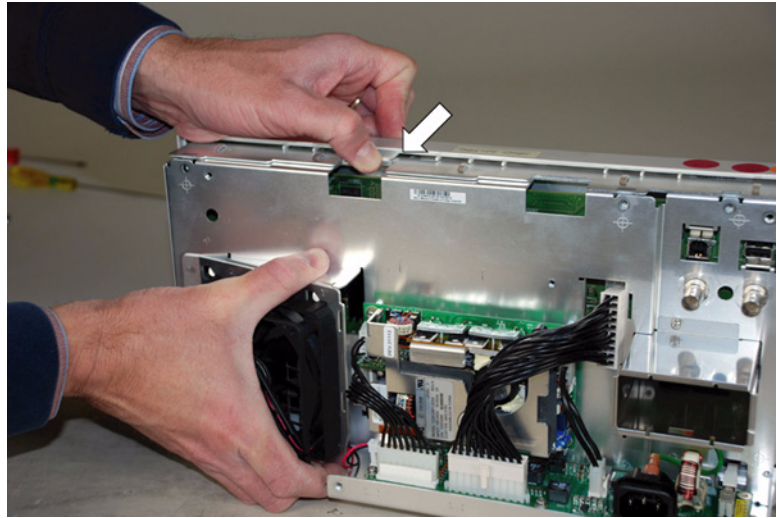


**Figure 34** Lifting front bezel latch



- b Carefully separate the rear deck from the front deck. Take care not to damage the extender switch.

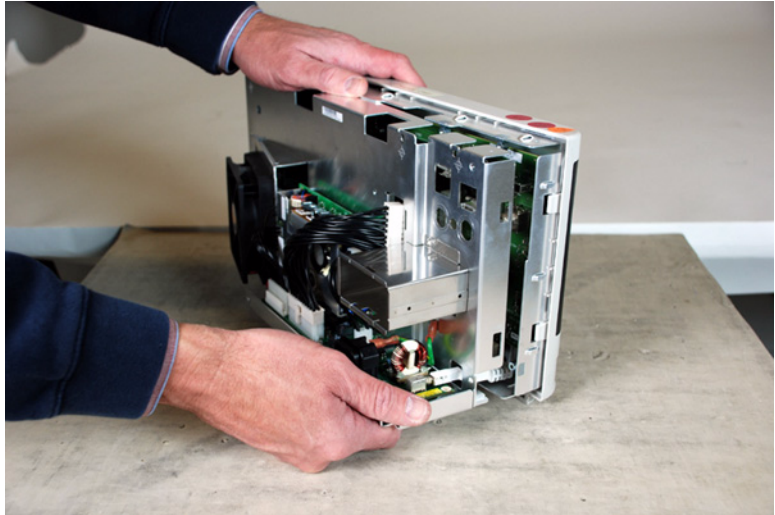

**Figure 35** Separating the rear and front decks

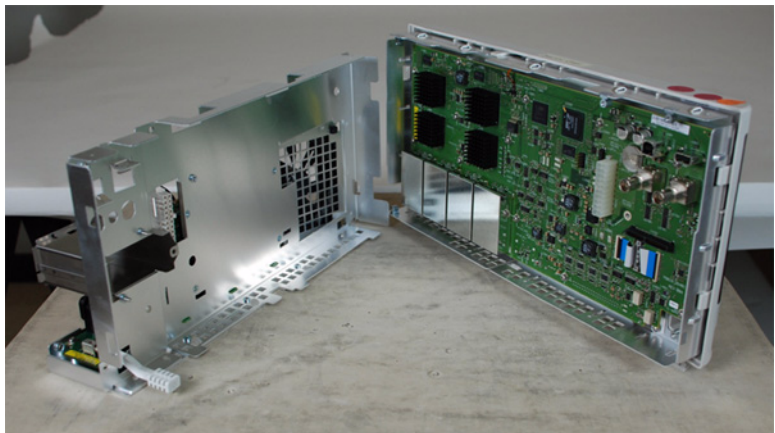


**Figure 36** Rear and front decks separated



## To remove the acquisition board

These steps describes how to remove the acquisition board.

- 1 Using a TORX T6 driver, locate and remove the 4 screws on the front of the instrument (4 Channel version).

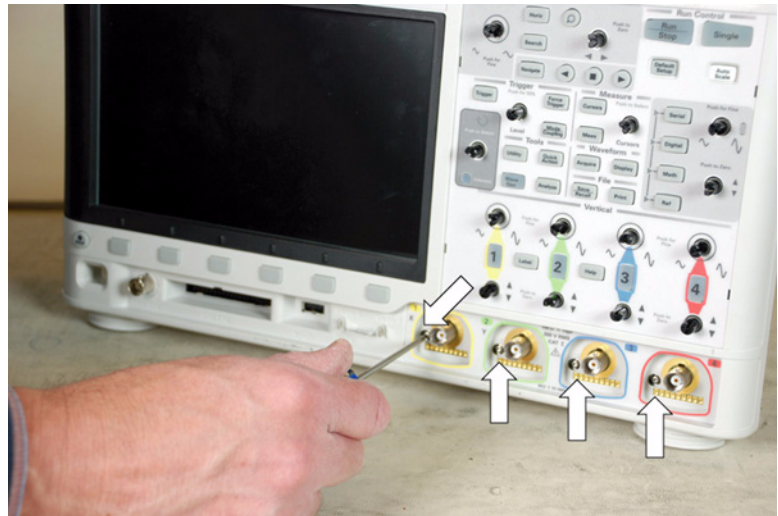


**Figure 37** Removing the T6 screws (4 channel version)

## 5 Replacing Assemblies


- 2 Disconnect keyboard, display, and display backlight power cables.

For the keyboard and display cables, flip up the connector clamp; then, slide the ribbon cables out.

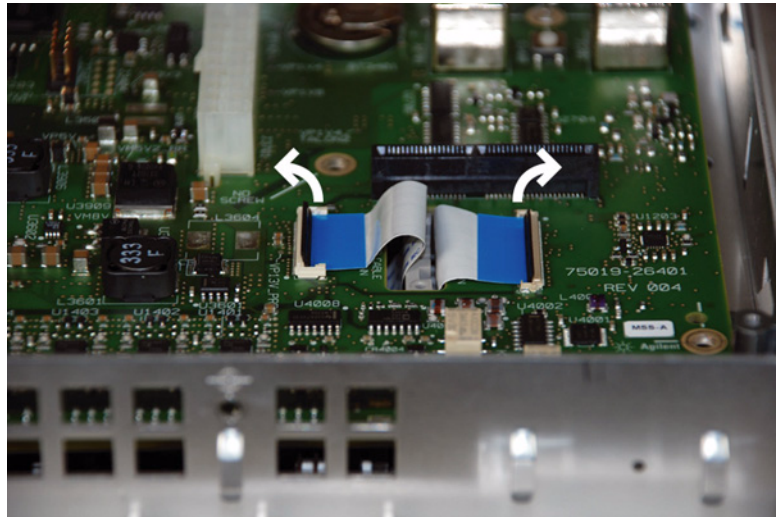

**Figure 38** Disconnecting keyboard and display cables from acquisition board


For the display backlight power cable, slide the connector clamp toward the top of the acquisition board; then, slide the ribbon cable out.

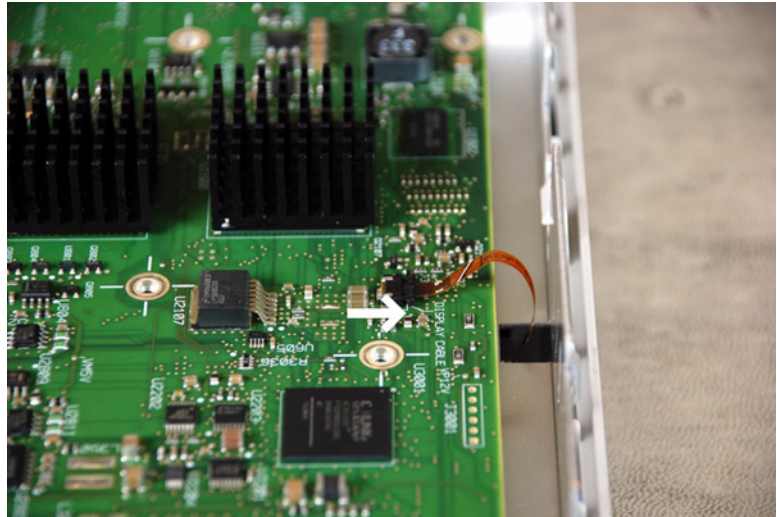

**Figure 39** Disconnecting display backlight power cable from acquisition board


## 5 Replacing Assemblies

- 3 Using a TORX T10 driver, locate and remove 13 mounting screws.

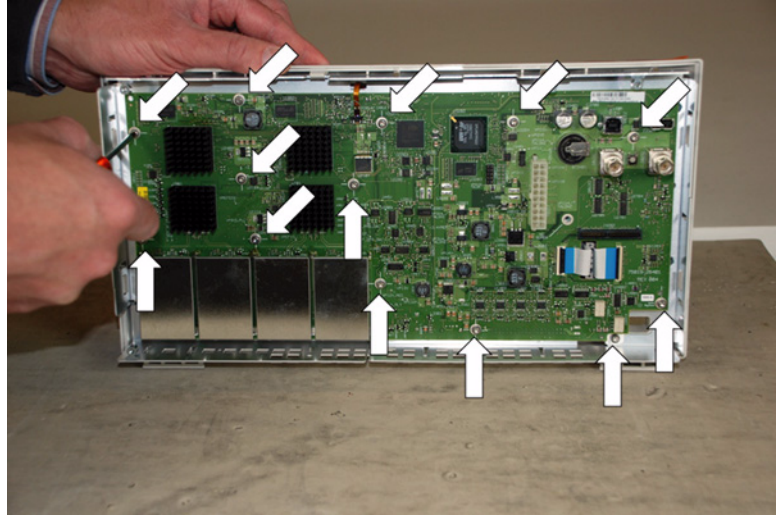

**Figure 40** Acquisition board mounting screw locations

- 4 Carefully lift the acquisition board off the front deck.

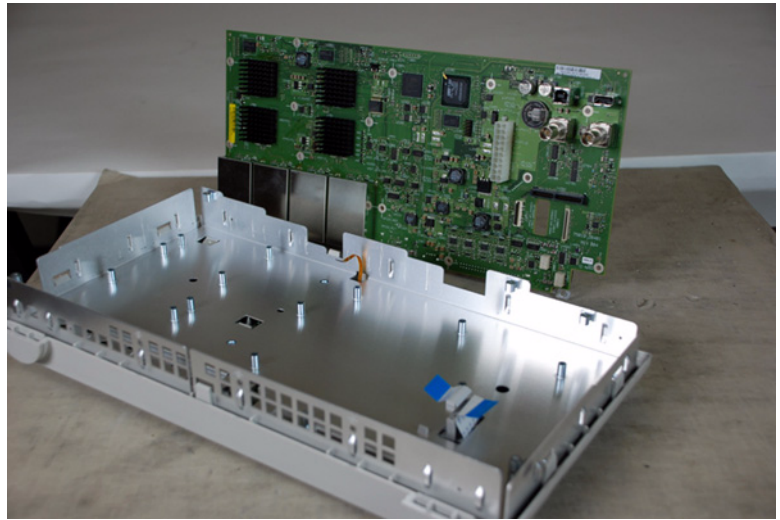

**Figure 41** Acquisition board removed from front deck

## To remove the front panel assembly

**WARNING**


Thin sheet metal parts may have sharp edges. Handle with care to avoid injury.

---


- 1 Remove the bezel from the front deck.

The bezel is secured to front deck by molded-in retaining clips located around the perimeter of the bezel.

Gently pry the retaining clips outward (either by hand or using a flat head screwdriver). Work your way around the bezel, releasing the clips and gently lifting the front deck away from the bezel.

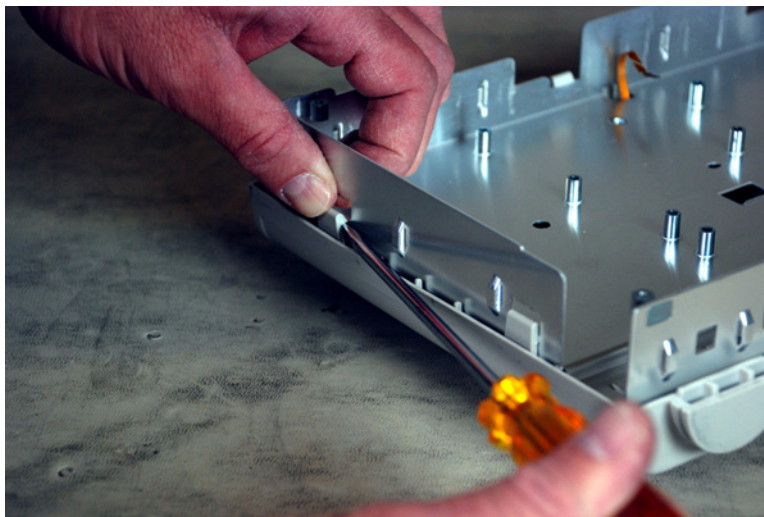

**Figure 42** Release the bezel clips from the front deck

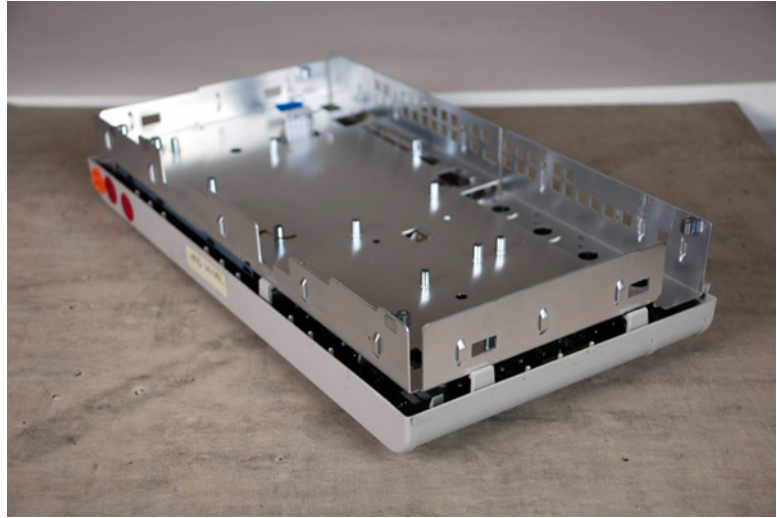

**Figure 43** All bezel clips released




**Figure 44** HINT: When reinstalling bezel, align ground terminal first



## 5 Replacing Assemblies


- 2 When all the bezel clips are released, gently lift the front deck away from the bezel, and disconnect the keyboard cable.

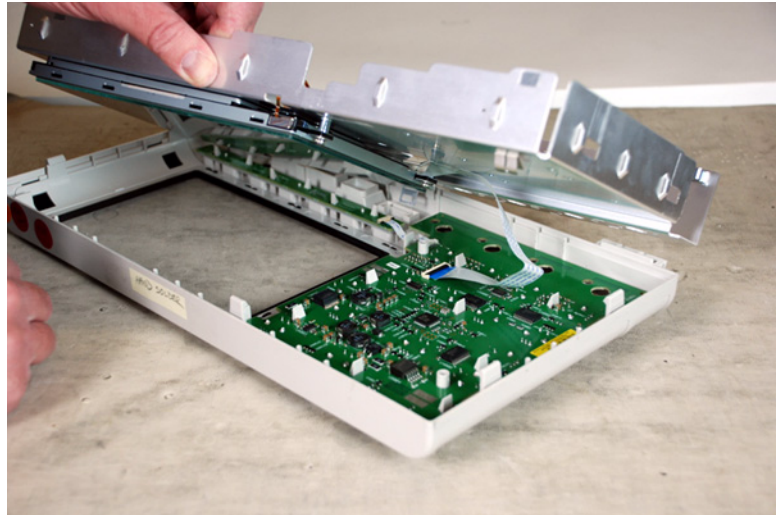

**Figure 45** Gently lift front deck from bezel



Flip up the keyboard cable connector clamp; then, slide the ribbon cable out.

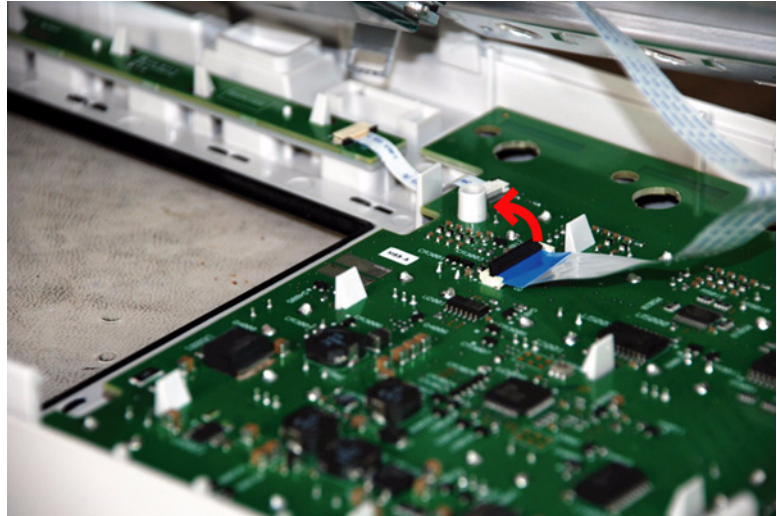


**Figure 46** Disconnect the keyboard cable

**3** Remove the softkey board cable from the keyboard board.

## 5 Replacing Assemblies

Slide the connector clamp toward the softkey board; then, slide the ribbon cable out.

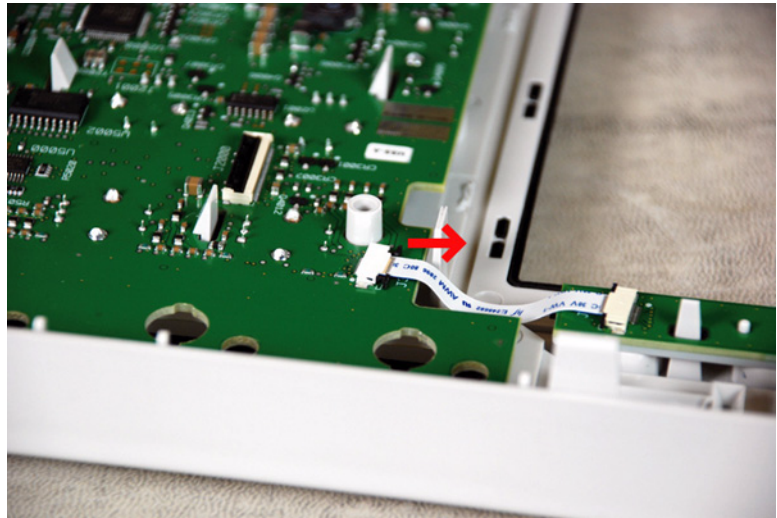

**Figure 47** Disconnect the softkey board cable

- 4 To separate the softkey board from the bezel, carefully pull back locking tabs that secure it.




**Figure 48** Unclip the softkey board from the bezel



**Figure 49** Remove the softkey keypad from the bezel

## 5 Replacing Assemblies

- 5 To separate the keyboard board from the bezel, carefully pull back locking tabs that secure it.

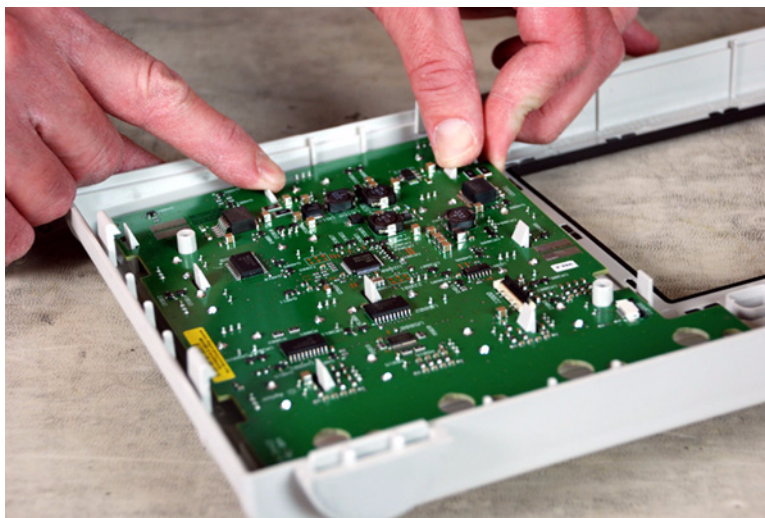

**Figure 50** Unclip the keyboard board from the bezel



**Figure 51** Remove the keyboard keypad from the bezel


## To remove the display assembly

The display assembly is part of the front panel assembly. Before you can remove and replace the display assembly, you must remove the front panel assembly. See [“To remove the front panel assembly”](#) on page 122.

**WARNING**

Thin sheet metal parts may have sharp edges. Handle with care to avoid injury.

- 1 Using a TORX T10 remove the four screws that secure the display to the front deck.

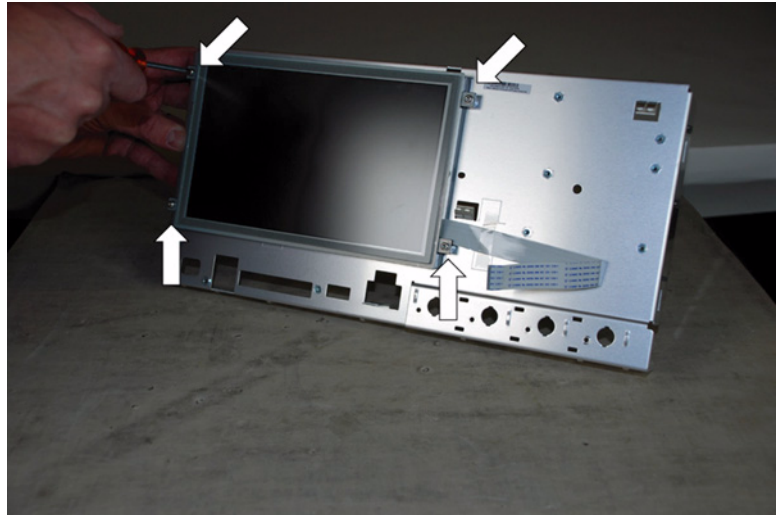


**Figure 52** Removing the display assembly



## 5 Replacing Assemblies

Take care while threading display cables thru front deck sheet metal openings.

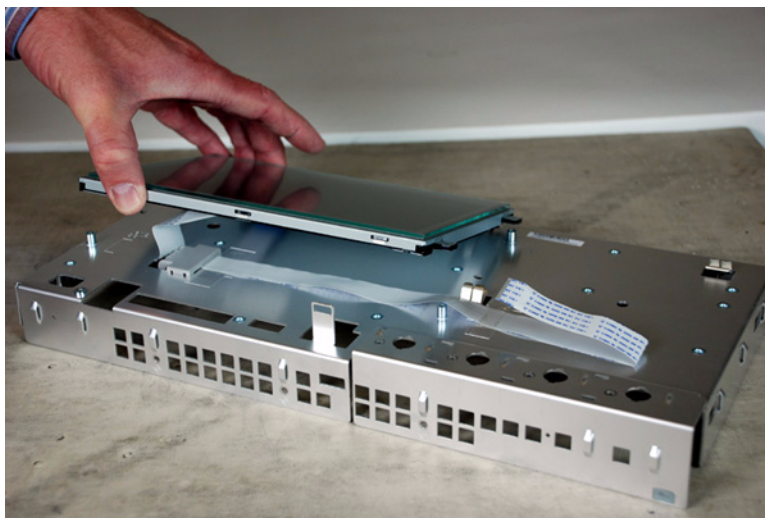

**Figure 53** Display assembly removed

## Replacing a 75019-68712 Display Assembly

Some 3000 X-Series oscilloscopes have the 75019-68712 display assembly.



**Figure 54** The 75019-68712 display assembly has a bracket under two of the retaining screws


If the 75019-68712 display assembly needs to be replaced, it is replaced with:

- 75019-68707 display assembly.
- 75019-47103 cable guide (inserted into the front deck to separate the display and keyboard cables).
- Also, you must retrieve the 40-pin display cable (75019-61606) from the 75019-68712 display assembly and reuse it with the 75019-68707 display assembly.

(The smaller display backlight power cable is already part of the 75019-68707 assembly.)

**To retrieve the 40-pin display cable**


- 1 Once the 75019-68712 display assembly has been removed, use a TORX T10 remove the two screws that secure the display to its mounting bracket.

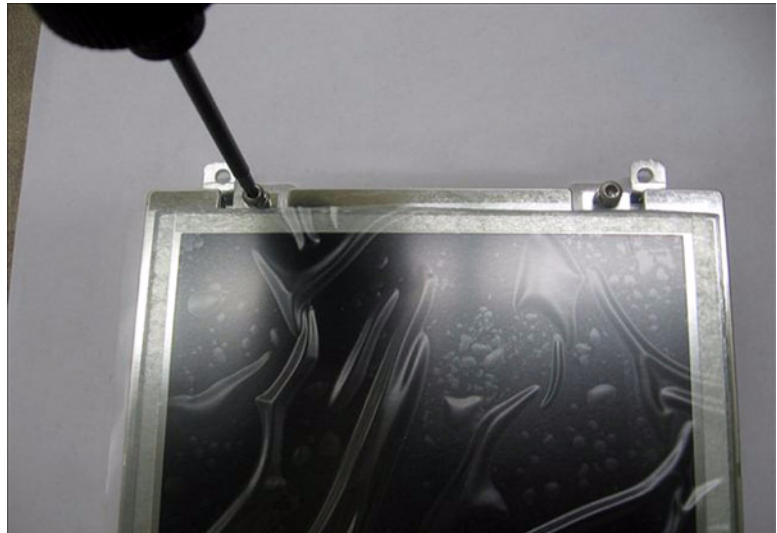

**Figure 55** Disassembling the 75019-68712 display assembly


- 2 Carefully separate the upper and lower halves of the display mounting bracket.



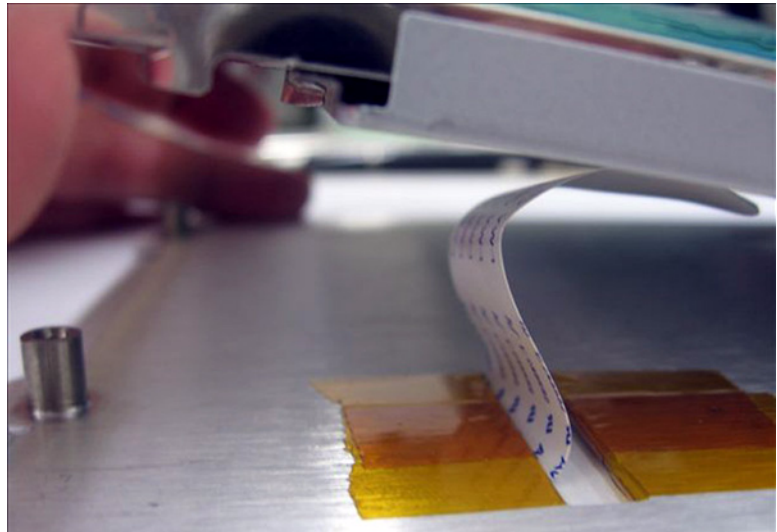

**Figure 56** Separating the 75019-68712 display mounting bracket

- 3 Flip-up the 40-pin connector's lid and remove the 75019-61606 display cable.

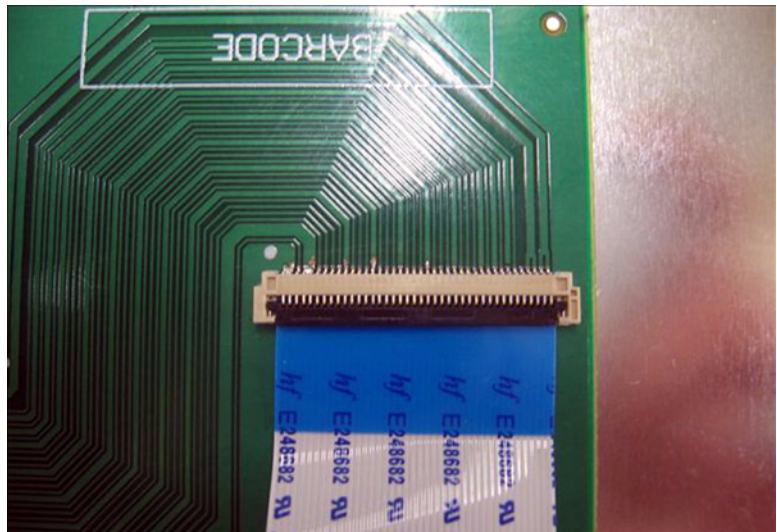

**Figure 57** Removing the 75019-61606 display cable

## To remove the fan assembly


- 1 Ensure that fan power cable has been disconnected from acquisition board.



**Figure 58** Disconnecting fan power cable

- 2 Carefully slide fan assembly (fan and fan mount) to the right, then lift away from rear deck.


Note, fan mount is soft and can be damaged by sharp sheet metal edges. Take care that the fan power cable is not damaged when pulling across sheet metal edges.

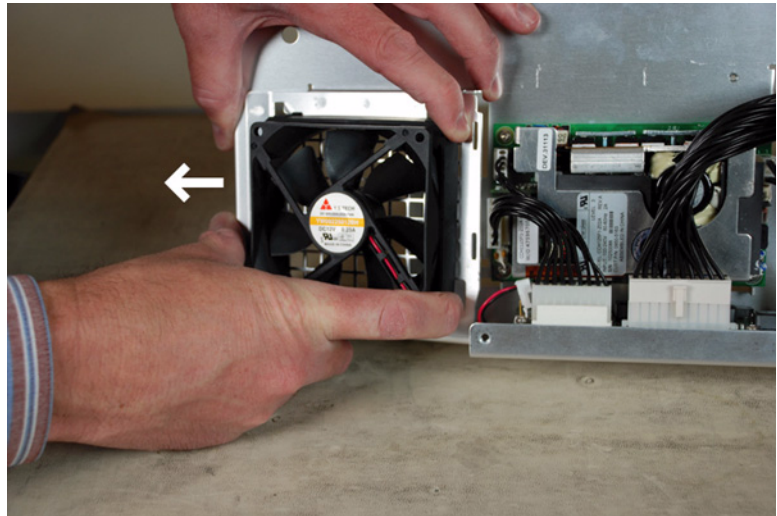


**Figure 59** Removing fan assembly

## To remove the power supply

- 1 Disconnect all cables from power supply board.

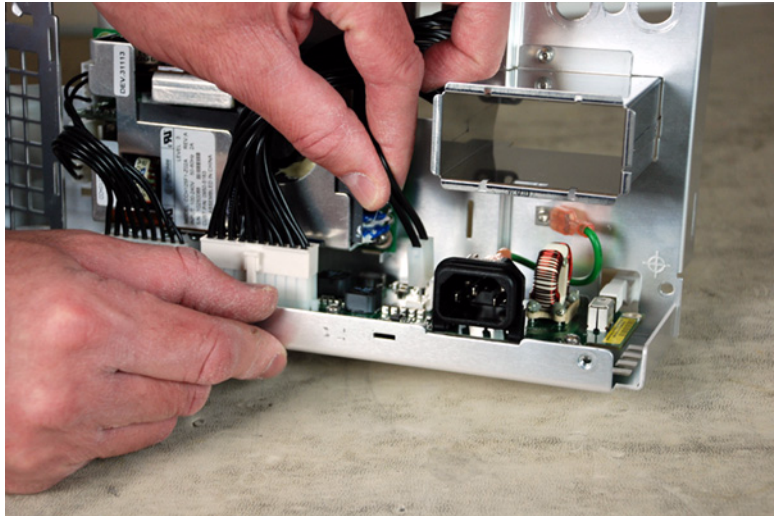

**Figure 60** Disconnecting the AC cable

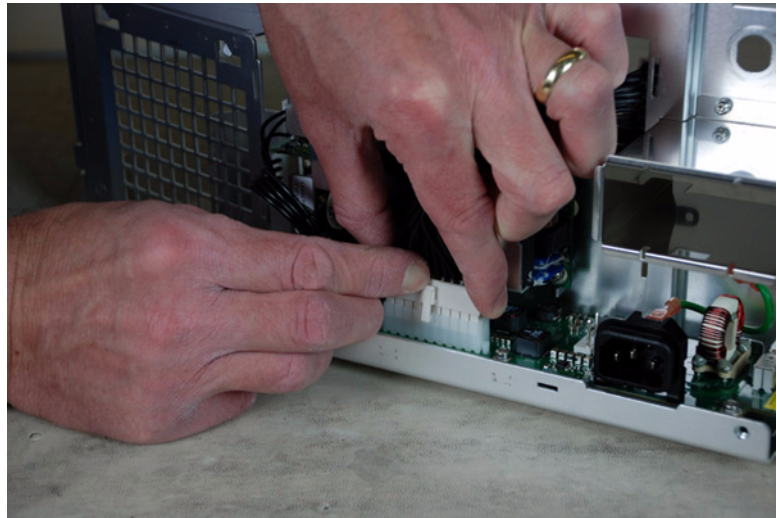

**Figure 61** Disconnecting the interboard supply cable from the line filter board




**Figure 62** Disconnecting the DC cable from the line filter board



## 5 Replacing Assemblies


- 2 Using a TORX T10 driver, locate and remove the four screws securing the power supply assembly to the rear deck.

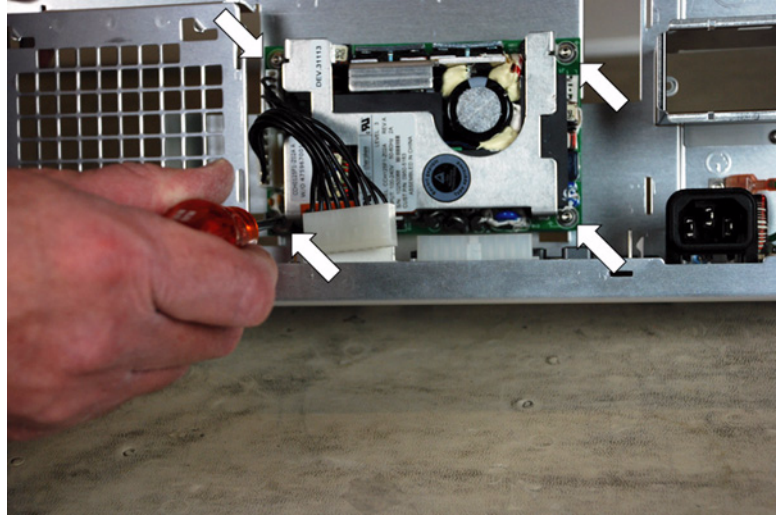

**Figure 63** Removing the power supply

## To remove the line filter board


- 1 Disconnect all cables on the line filter board.
- 2 Remove the option module guide.

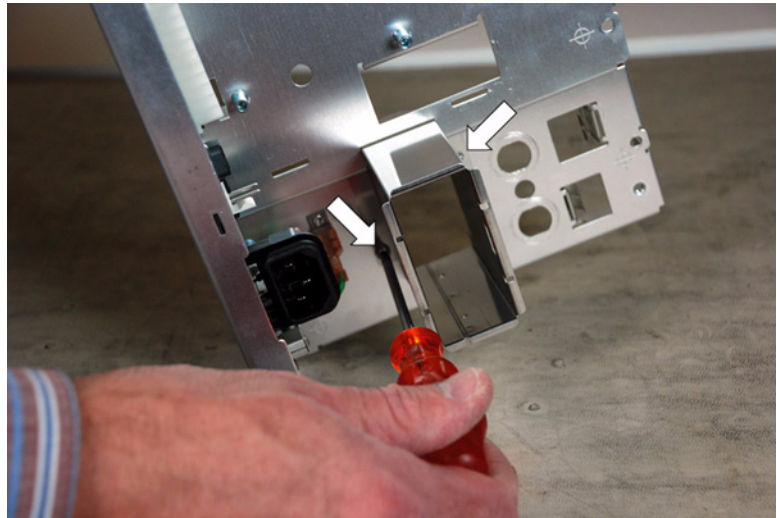

**Figure 64** Removing the option module guide

## 5 Replacing Assemblies


3 Disconnect the ground wire from its chassis terminal.

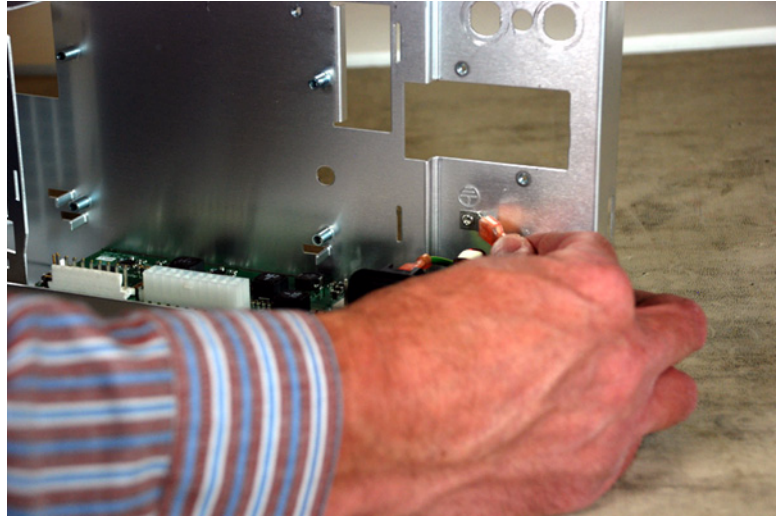

**Figure 65** Disconnecting the ground wire



- 4 Using a TORX T10 driver, locate and remove the three screws securing the line filter board to the rear deck.

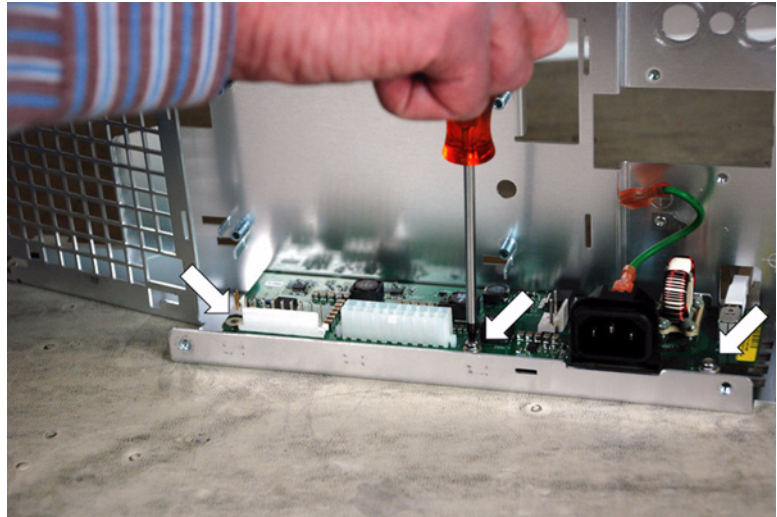


**Figure 66** Removing the line filter board screws

## 5 Replacing Assemblies

- 5 Slide the line filter board out of the slots in the rear deck.

Take care that you do not damage the switch extender during removal.

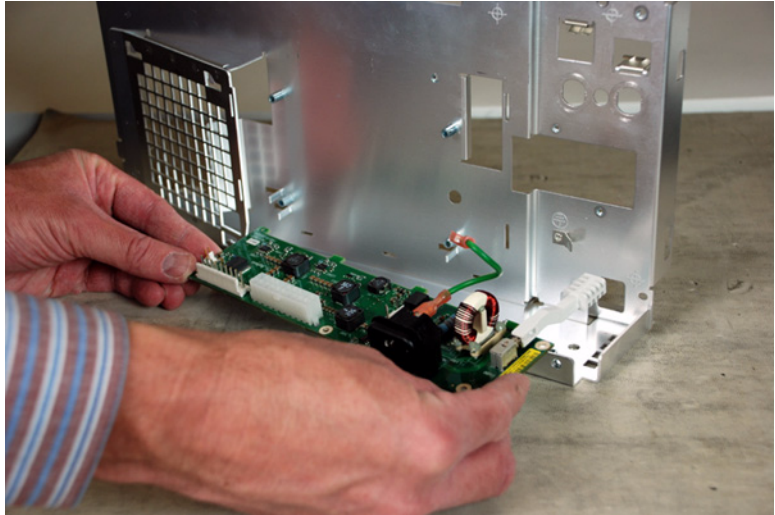


**Figure 67** Removing the line filter board

- 6 To remove the switch extender, gently pry open the extender using a flat head screwdriver.

**CAUTION**

Twisting the latch too much could cause it to break!

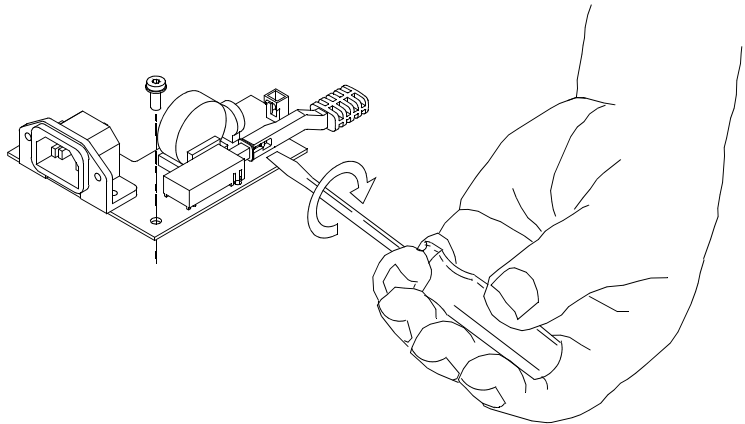

**Figure 68** Removing the power switch extender

## **5 Replacing Assemblies**



## 6 Replaceable Parts

This chapter describes how to order replaceable assemblies and parts for the Agilent 2000/3000 X-Series oscilloscopes.

Diagrams and parts lists are included for assemblies and hardware that you can order.

Before working on the oscilloscope, read the safety summary at the back of this book.



## Ordering Replaceable Parts

### Listed Parts

To order a part in the parts list, quote the Agilent Technologies part number, indicate the quantity desired, and address the order to the nearest Agilent Technologies Sales Office. To find your nearest sales office go to [www.agilent.com](http://www.agilent.com).

### Unlisted Parts

To order a part not listed in the parts list, include the instrument part number, instrument serial number, a description of the part (including its function), and the number of parts required. Address the order to the nearest Agilent Technologies Sales Office.

### Direct Mail Order System

Within the USA, Agilent Technologies can supply parts through a direct mail order system. There are several advantages to this system:

- Direct ordering and shipping from the Agilent Technologies parts center in California, USA.
- No maximum or minimum on any mail order. (There is a minimum amount for parts ordered through a local Agilent Technologies Sales Office when the orders require billing and invoicing.)
- Prepaid transportation. (There is a small handling charge for each order.)
- No invoices.

In order for Agilent Technologies to provide these advantages, please send a check or money order with each order.

Mail order forms and specific ordering information are available through your local Agilent Technologies Sales Office. Addresses and telephone numbers are located in a separate document shipped with the manuals.


## Exchange Assemblies

Some parts used in this instrument have been set up for an exchange program. This program allows the customer to exchange a faulty assembly with one that has been repaired, calibrated, and performance-verified by the factory. The cost is significantly less than that of a new part. The exchange parts have a part number in the form XXXXX-695XX.

After receiving the repaired exchange part from Agilent Technologies, a United States customer has 30 days to return the faulty assembly. For orders not originating in the United States, contact the local Agilent Technologies service organization. If the faulty assembly is not returned within 30 days, the customer will be charged an additional amount. The additional amount will be the difference in price between a new assembly and that of an exchange assembly.


## Exploded Views

The following exploded views provide a graphical representation of the oscilloscope at the time this manual was released. Not all parts are shown. Your parts may be slightly different than those shown. These views provide reference designator numbers that map to those used in the parts list table in this chapter.

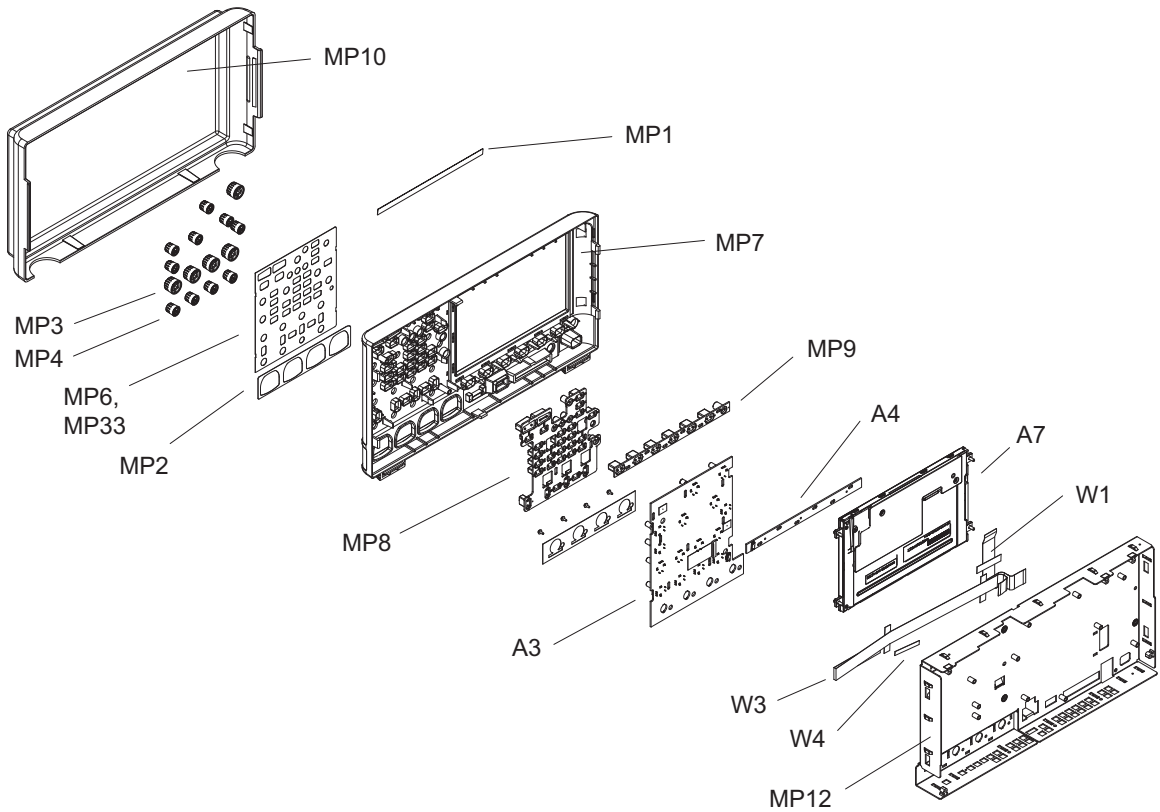

**Figure 69** Exploded View 1 of 2



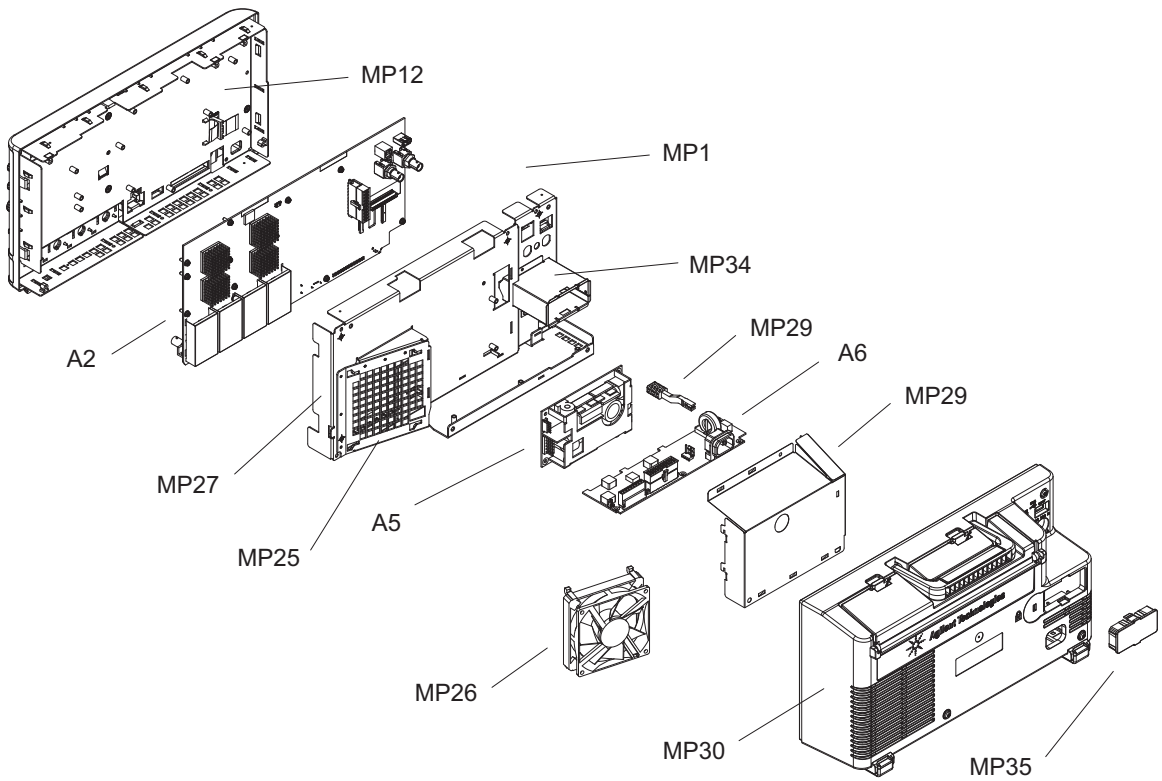

**Figure 70** Exploded View 2 of 2

## Replaceable Parts List

The information given for each part consists of the following:

- Reference designation.
- Agilent Technologies part number.
- Total quantity (Qty) in the instrument or on assembly.
- Description of the part.

**Table 18** Replaceable Parts

Ref Des	Agilent Part Number	Qty	Description
	75014-68801	1	Oscilloscope 2000 X-Series 2-Ch - 70, 100, 200 MHz
	75014-69801	1	Oscilloscope 2000 X-Series 2-Ch - 70, 100, 200 MHz (exchange)
	75015-68801	1	Oscilloscope 2000 X-Series 4-Ch - 70, 100, 200 MHz
	75015-69801	1	Oscilloscope 2000 X-Series 4-Ch - 70, 100, 200 MHz (exchange)
	75016-68801	1	Oscilloscope 3000 X-Series 2-Ch - 100, 200 MHz
	75016-69801	1	Oscilloscope 3000 X-Series 2-Ch - 100, 200 MHz (exchange)
	75017-68801	1	Oscilloscope 3000 X-Series 4-Ch - 100, 200 MHz
	75017-69801	1	Oscilloscope 3000 X-Series 4-Ch - 100, 200 MHz (exchange)
A2	75018-66503	1	Acquisition board 3000 X-Series 2-Ch - 350, 500 MHz
A2	75018-69503	1	Acquisition board 3000 X-Series 2-Ch - 350, 500 MHz (exchange)
A2	75019-66503	1	Acquisition board 3000 X-Series 4-Ch - 350, 500 MHz
A2	75019-69503	1	Acquisition board 3000 X-Series 4-Ch - 350, 500 MHz (exchange)
A2	75022-66501	1	Acquisition board 3000 X-Series 2-Ch - 1 GHz
A2	75022-69501	1	Acquisition board 3000 X-Series 2-Ch - 1 GHz (exchange)
A2	75023-66501	1	Acquisition board 3000 X-Series 4-Ch - 1 GHz
A2	75023-69502	1	Acquisition board 3000 X-Series 4-Ch - 1 GHz (exchange)

**Table 18** Replaceable Parts (continued)

Ref Des	Agilent Part Number	Qty	Description
A3	75019-66422	1	PCA - 2 Channel Keyboard 3000 X-Series
A3	75019-66423	1	PCA - 4 Channel Keyboard 3000 X-Series
A4	75015-66427	1	PCA - Keyboard Entry Softkey Board
A5	0950-5277	1	Power Supply Switching AC/DC 125W
A6	75019-66424	1	PCA - Line Filter Board
A7	75019-68707 75019-68712	1	Display assembly. A defective 75019-68712 is replaced with 75019-68707 and the 75019-47103 cable guide. See <a href="#">"Replacing a 75019-68712 Display Assembly"</a> on page 131.
H2	54684-42202	2	Hole plug front panel (2 Channel only, not shown)
H5	2950-0054	3	Nut, 1/2-28 THD (secures BNCs, not shown)
H11	2190-0068	3	Washer-LK Intl T 1/2 In. .505 IN-ID (for BNCs, not shown)
H3	0515-0374	37	Screw-Machine with Crest-Cup-Con-Washer Pan-HD Torx-T10 M3X0.5 10mm-LG SST-300 Passivated (not shown)
H4	0515-0658	4, 8	Screw-Machine w/Crest-Cup-Con-Wshr Pan-HD TORX-T6 M2X0.4 6mm-LG SST-300 Passivated (not shown, qty=4 for 2 Ch, qty=8 for 4 Ch)
H6	0515-0380	4	Screw-Machine W/Crest-Cup-Con-Washer Pan-HD Torx-T20 M4X0.7 10mm-LG SST-300 Passivated (not shown)
H7	0515-1753	3	Screw-Machine with Patch-Lock Pan-HD Torx-T10 M3X0.5 8mm-LG SST-300 Passivated (not shown)
MP1	75010-94301	1	ID Label DSO-X 2002A
MP1	75010-94302	1	ID Label MSO-X 2002A
MP1	75011-94301	1	ID Label DSO-X 2004A
MP1	75011-94302	1	ID Label MSO-X 2004A
MP1	75012-94301	1	ID Label DSO-X 2012A
MP1	75012-94302	1	ID Label MSO-X 2012A

## 6 Replaceable Parts

**Table 18** Replaceable Parts (continued)

Ref Des	Agilent Part Number	Qty	Description
MP1	75013-94301	1	ID Label DSO-X 2014A
MP1	75013-94302	1	ID Label MSO-X 2014A
MP1	75014-94301	1	ID Label DSO-X 2022A
MP1	75014-94302	1	ID Label MSO-X 2022A
MP1	75015-94301	1	ID Label DSO-X 2024A
MP1	75015-94302	1	ID Label MSO-X 2024A
MP1	75016-94303	1	ID Label DSO-X 3012A
MP1	75016-94304	1	ID Label MSO-X 3012A
MP1	75017-94303	1	ID Label DSO-X 3014A
MP1	75017-94304	1	ID Label MSO-X 3014A
MP1	75019-94308	1	ID Label DSO-X 3024A
MP1	75019-94309	1	ID Label MSO-X 3024A
MP1	75016-94301	1	ID Label DSO-X 3032A
MP1	75016-94302	1	ID Label MSO-X 3032A
MP1	75017-94301	1	ID Label DSO-X 3034A
MP1	75017-94302	1	ID Label MSO-X 3034A
MP1	75018-94301	1	ID Label DSO-X 3052A
MP1	75018-94302	1	ID Label MSO-X 3052A
MP1	75019-94301	1	ID Label DSO-X 3054A
MP1	75019-94307	1	ID Label MSO-X 3054A
MP1	75022-94301	1	ID Label DSO-X 3102A
MP1	75022-94302	1	ID Label MSO-X 3102A
MP1	75023-94301	1	ID Label DSO-X 3104A
MP1	75023-94302	1	ID Label MSO-X 3104A

**Table 18** Replaceable Parts (continued)

Ref Des	Agilent Part Number	Qty	Description
MP2	75019-94304	1	BNC Label 2 Channel
MP2	75019-94305	1	BNC Label 4 Channel
MP3	75019-47401	5	Large Rotary Knob
MP4	75019-47402	10	Small Rotary Knob
MP6	75019-94302	1	Front Keyboard Label 2 Channel
MP6	75019-94303	1	Front Keyboard Label 4 Channel
MP7	75019-60201	1	Panel Bezel Assembly
MP8	75019-41901	1	Keyboard Keypad
MP9	75019-41902	1	Softkey Keypad
MP12	75019-00101	1	Front Deck
MP14	75019-47103	1	Cable Guide
MP27	75019-00102	1	Rear Deck
MP25	75019-44701	1	Fan Mount
MP26	3160-4343	1	Fan
MP28	75019-43901	1	Extender, Power Switch
MP29	75019-00602	1	Power Supply Shield
MP30	75019-64401	1	Bucket Assembly

## 6 Replaceable Parts

**Table 18** Replaceable Parts (continued)

Ref Des	Agilent Part Number	Qty	Description
MP33	75019-94310	*	Overlay - Traditional Chinese, 4 channel
MP33	75019-94330	*	Overlay - Traditional Chinese, 2 channel
MP33	75019-94312	*	Overlay - Japanese, 4 channel
MP33	75019-94311	*	Overlay - Japanese, 2 channel
MP33	75019-94315	*	Overlay - Russian, 4 channel
MP33	75019-94322	*	Overlay - Russian, 2 channel
MP33	75019-94316		Overlay - French, 4 channel
MP33	75019-94324	*	Overlay - French, 2 channel
MP33	75019-94317	*	Overlay - Spanish, 4 channel
MP33	75019-94325	*	Overlay - Spanish, 2 channel
MP33	75019-94318	*	Overlay - German, 4 channel
MP33	75019-94326	*	Overlay - German, 2 channel
MP33	75019-94319	*	Overlay - Portuguese, 4 channel
MP33	75019-94327	*	Overlay - Portuguese, 2 channel
MP33	75019-94320	*	Overlay - Simplified Chinese, 4 channel
MP33	75019-94328	*	Overlay - Simplified Chinese, 2 channel
MP33	75019-94321	*	Overlay - Korean, 4 channel
MP33	75019-94329	*	Overlay - Korean, 2 channel
MP33	75019-94331	*	Overlay - Italian, 4 channel
MP33	75019-94323	*	Overlay - Italian, 2 channel
MP34	75019-00608	1	Guide - Option Module
MP35	75019-42203	1	Hole Plug - Option Module
W5	75019-61602	1	Cable - DC
W7	75019-61603	1	Cable - AC

**Table 18** Replaceable Parts (continued)

Ref Des	Agilent Part Number	Qty	Description
	75019-61604	1	Cable - Ground Wire
W4	75019-61605	1	Soft Keyboard Cable
W1	75019-61606	1	Cable - Display
W3	75019-61607	1	Keyboard Cable
	75019-61601	1	Cable Interboard Supply
W6	Power cord	0-1	Part number varies by country. Contact your local Agilent sales office for replacement.
	N2862B	*	Passive Probe 10:1, 150 MHz
	N2863B	*	Passive Probe 10:1, 300 MHz
	N2890A	*	Passive Probe 10:1, 500 MHz
MP10	75019-44108	*	Protective Cover Assembly
Not shown	75019-68705	*	LAN Module
Not shown	75019-68706	*	GPIB Module
Not shown	N6456-60001	*	Rack Mount Kit for 2000/3000 X-Series Oscilloscope

\*Optional item.







## 7 Safety Notices

This apparatus has been designed and tested in accordance with IEC Publication 1010, Safety Requirements for Measuring Apparatus, and has been supplied in a safe condition. This is a Safety Class I instrument (provided with terminal for protective earthing). Before applying power, verify that the correct safety precautions are taken (see the following warnings). In addition, note the external markings on the instrument that are described under “Safety Symbols.”

### Warnings

Before turning on the instrument, you must connect the protective earth terminal of the instrument to the protective conductor of the (mains) power cord. The mains plug shall only be inserted in a socket outlet provided with a protective earth contact. You must not negate the protective action by using an extension cord (power cable) without a protective conductor (grounding). Grounding one conductor of a two-conductor outlet is not sufficient protection.

Only fuses with the required rated current, voltage, and specified type (normal blow, time delay, etc.) should be used. Do not use repaired fuses or short-circuited fuseholders. To do so could cause a shock or fire hazard.

## Safety Notices

If you energize this instrument by an auto transformer (for voltage reduction or mains isolation), the common terminal must be connected to the earth terminal of the power source.

Whenever it is likely that the ground protection is impaired, you must make the instrument inoperative and secure it against any unintended operation.

Service instructions are for trained service personnel. To avoid dangerous electric shock, do not perform any service unless qualified to do so. Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

Do not install substitute parts or perform any unauthorized modification to the instrument.

Capacitors inside the instrument may retain a charge even if the instrument is disconnected from its source of supply.

Do not operate the instrument in the presence of flammable gasses or fumes. Operation of any electrical instrument in such an environment constitutes a definite safety hazard.

Do not use the instrument in a manner not specified by the manufacturer.

## To clean the instrument

If the instrument requires cleaning: (1) Remove power from the instrument. (2) Clean the external surfaces of the instrument with a soft cloth dampened with a mixture of mild detergent and water. (3) Make sure that the instrument is completely dry before reconnecting it to a power source.

## Safety Symbols



Instruction manual symbol: the product is marked with this symbol when it is necessary for you to refer to the instruction manual in order to protect against damage to the product.



Hazardous voltage symbol.



Earth terminal symbol: Used to indicate a circuit common connected to grounded chassis.

## Safety Notices

# Index

## A

- accuracy, DC vertical gain, 35
- accuracy, dual cursor, 42
- Agilent
  - contact information, 21
- assemblies
  - exchange, 147
  - replacing, 101

## B

- bandwidth
  - verification, 49

## C

- cabinet, removing, 104
- calibration, 69
- cautions, 84, 87, 90, 102, 103, 138
- certificate of calibration, 69
- channels
  - problem solving, 76
- cleaning the instrument, 158
- compensating your probe, 81
- connecting for threshold test, 32
- contact Agilent, 21

## D

- DC vertical gain accuracy, 35
- digital channel
  - testing, 29
  - verification, 30
- digital channels, 4
- display
  - assembly removal, 122, 129
  - problem solving, 74
- dual cursor accuracy, 42

## E

- equipment, test, 25
- exchange assemblies, 147
- exploded view
  - front panel, 148
  - instrument, 149

## F

- fan assembly removal, 134
- front panel
  - exploded view, 148
  - removal, 110
- front panel self test, 78

## H

- hardware self test, 78

## I

- internal self-tests, 78

## K

- keyboard, removal, 117

## L

- LED, startup sequence, 77
- lid, removal, 105
- line filter board removal, 139

## M

- making test connector, 27
- measurement category, 17
  - definitions, 17

## N

- NIST, 69

## O

- ordering parts, 146
- overvoltage category, 19

## P

- parts
  - list, 150
  - ordering, 146
- passive probe, 155
- perform user cal, 69
- performance
  - test record, 63, 65
- pollution degree, 19
- pollution degree, definitions, 19
- power
  - cord list, 155
  - supply removal, 136
  - supply shield, removal, 107
  - test points, 88, 89
- power requirements, 16
- probe
  - N2862B, 155
  - N2863B, 155
  - N2890A, 155
- probes
  - compensating, 81
- problem solving, 73

## R

- record tests, 63, 65

## Index

remove, 139  
  cabinet, 104  
  display assembly, 122, 129  
  fan assembly, 134  
  front panel, 110  
  keyboard, 117  
  power supply, 136  
  power supply shield, 107  
  storage lid, 105  
replaceable parts list, 150  
replacing assemblies, 101  
run self-tests, 78

## S

safety notice, 67, 84  
self test, front panel, 78  
self test, hardware, 78  
self-alignment, user cal, 69  
self-tests, 78  
specifications, 20  
startup sequence, 77  
status, User Cal, 72  
status, user cal, 69  
storage lid, removal, 105

## T

test  
  connector, constructing, 27  
  digital channels, 29  
  equipment, 25  
  points, power, 88, 89  
  record, 63, 65  
threshold  
  accuracy, digital channel, 30  
  test diagram, 32  
trace display  
  problem solving, 75  
transient withstand capability, 18  
trigger  
  sensitivity, 57  
  sensitivity, external, 60  
  sensitivity, internal, 58

troubleshooting, 73  
  equipment required, 83  
  fan, 99  
  flowchart, 87  
  power supply, 90

## U

user calibration, 69

## V

verify  
  bandwidth, 49  
  digital channel, 30  
  trigger, 57

## W

warnings, 102  
warranted specifications, 20