




HEWLETT
PACKARD

MODULATION
ANALYZER
150 kHz - 1800 MHz



Technical Data 1 July 1982

Outstanding Signal Characterization

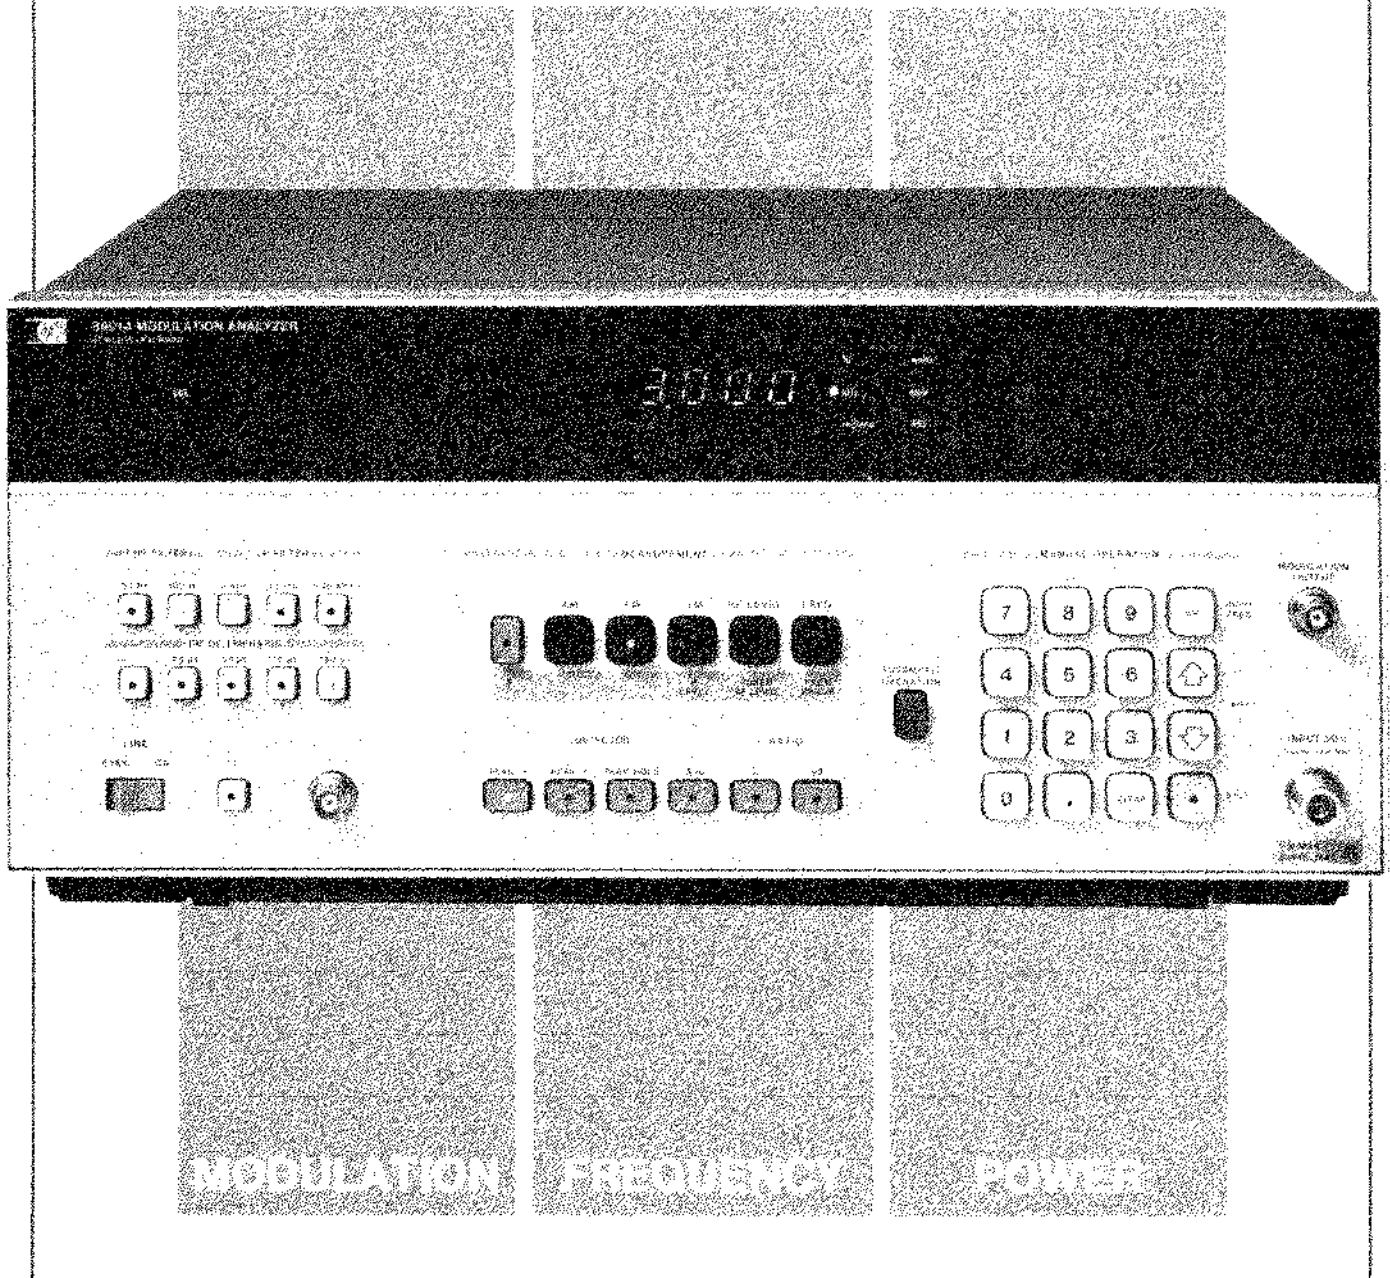

MEASUREMENTS

Frequency

Range: 150 kHz to 1,000 MHz.

Resolution: 10 Hz below 1000 MHz, 100 Hz above 1000 MHz.

Input Level: Automatic Mode: -20 dBm to $+30$ dBm.
Manual Mode: Typically -60 dBm to $+30$ dBm.

Power

Display: Peak envelope power.

Range: 1 milliwatt to 1 watt.

Accuracy: ± 1.5 dB

Input Power Protection:
 > 25 watts.

Modulation

FREQUENCY MODULATION

Rates: 20 Hz to 200 kHz.

Deviations: to 400 kHz.

Accuracy: $\pm 1\%$ of reading ± 1 digit for rates 30 Hz to 100 kHz.

AMPLITUDE MODULATION

Rates: 20 Hz to 100 kHz.

Depths: to 99%.

Accuracy: $\pm 1\%$ of reading ± 1 digit for rates 50 Hz to 50 kHz and depths $> 5\%$.

PHASE MODULATION

Rates: 200 Hz to 20 kHz.

Deviations: to 400 radians.

Accuracy: $\pm 3\%$ of reading ± 1 digit.



Indicators display current HP-IB status. Local key returns Analyzer to front panel control to allow manual measurements.

Large LED display permits distant viewing.


Independently selectable high-pass and low-pass filters allow the user to match the post-detection bandwidth to his application.

Four standard de-emphasis networks are available for making FM measurements.

Pre-display key allows de-emphasis networks to be positioned either before or after the displayed measurement so actual or "de-emphasized" deviation can be displayed.

Optional calibrator provides extremely accurate AM and FM signals. AM depth and FM deviation are calibrated to 0.1% accuracy. This allows for easy self-check of Analyzer accuracy and accurate recalibration.


Keys select positive peak, negative peak, or average detectors for measuring modulation. Peak hold is used with either peak detector for measuring transients.

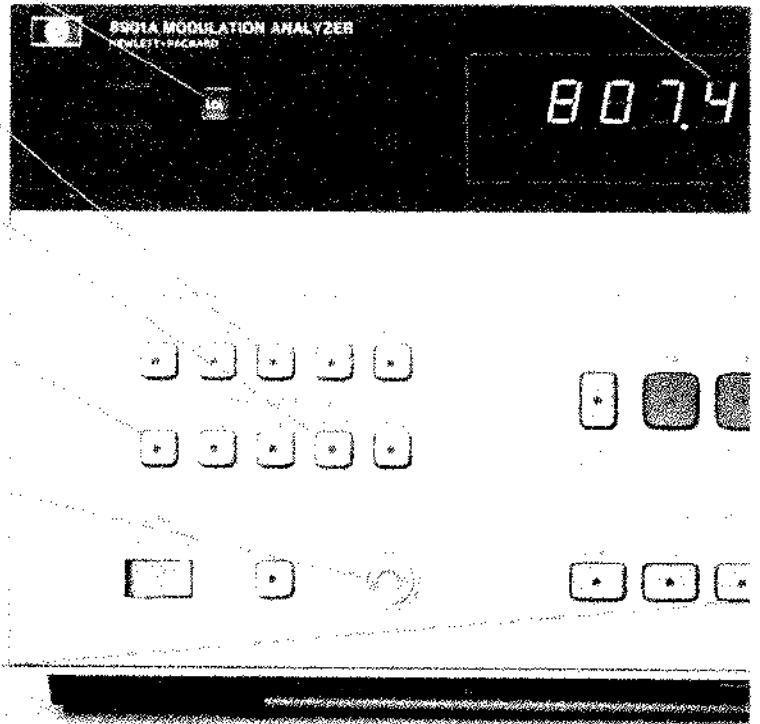

Recorder output provides a dc voltage proportional to the peak demodulated output voltage.

IF output can be used to view the amplitude modulated envelope with an oscilloscope or as an output for specialized detectors.

The 10 inps an external increase to noise.

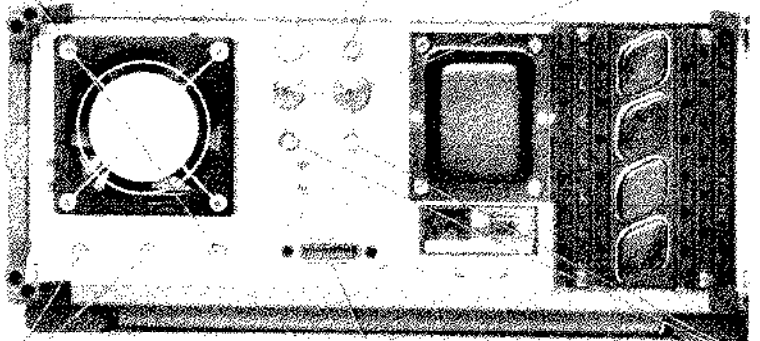

Connectors provide continuous output of dc coupled demodulated AM and FM.

HP-IB connector provides for output of measurement data and remote control of all functions.

10 MHz injected when is connects able on Cor erence.

Keys make measurement selection simple. LED's indicate which measurement is being made.

Limit indicator lights when measured value exceeds that entered by the operator.

Numerical keys are used for entering manually tuned frequencies, frequency increments, and special function codes.


Low distortion of the recovered modulation allows measurements such as modulation distortion or stereo separation.

Special function key allows complete control of Analyzer functions for increased capability. This key also executes many built-in service routines which speed trouble isolation.

Input circuitry is protected from damage due to excessive power for signals up to 25 watts.

In automatic operation the Analyzer automatically tunes to the largest input signal and autoranges for maximum resolution and accuracy.

Pull-out information card is quick reference for instrument operation, special functions, and error messages.

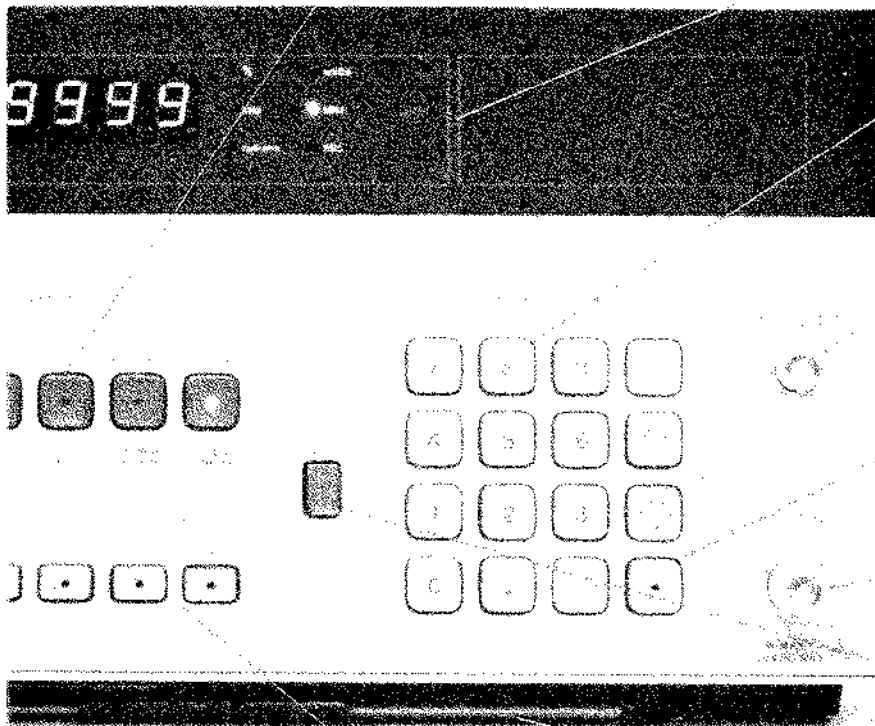

(Option 003) permits source to be used to tuning speed or reduce

Ratio keys allow all measurements to be displayed in dB or % relative to a measured or keyboard entered value.


It automatically selects external reference. Output is only available in 003, 1x10³ Hz ref.

Applications

Mobile Radio

The 8901A Modulation Analyzer combines all the capabilities necessary for making accurate transmitter measurements. It can be used in making all the tests listed below. It can also be used to test modules and subassemblies from either the transmitter or receiver. For reliability, input power protection reduces the chance of accidentally damaging the Modulation Analyzer by connecting it directly to a high power transmitter.


Carrier power	Incidental AM or FM
Carrier frequency and stability	Modulation limiting
AM depth	Instantaneous
FM deviation	Steady state
Hum and noise	Audio frequency response

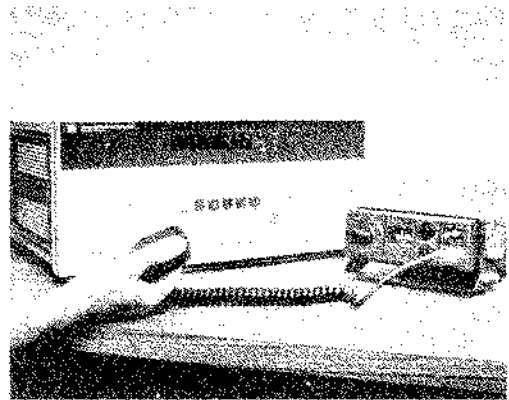

Maintenance and Metrology

Accurately measuring modulation has long been a problem for metrology laboratories. The 8901A Modulation Analyzer helps solve this problem two ways. First, it provides an extremely accurate method of measuring AM depth and FM deviation, and it recovers the modulation with little degradation for making measurements such as modulation distortion. Second, the optional calibrators provide a precise modulation source for calibration. There are many metrology and maintenance uses for the Modulation Analyzer. They include:


- Signal generator calibration
- Modulation calibration standard
- VCO and VCXO characterization

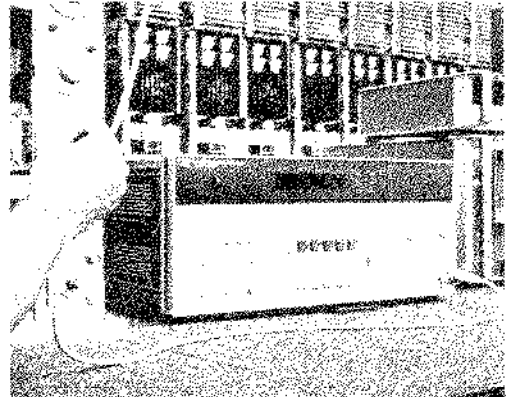

Research and Development

The accuracy and versatility of the Modulation Analyzer make it a very useful laboratory instrument for characterizing a wide variety of devices and assemblies. When used with a modulated signal source the Modulation Analyzer can make stimulus-response measurements for direct measurement of a device's effects on such signals. Because of its wide frequency range, it can measure the performance of both RF and IF assemblies. Characterizing modulated sources for sensitivity, distortion, and incidentals, and measuring the noise performance of local oscillators is also possible.

Mixer & Amplifier Compression	Incidental AM or FM
Local oscillator residual FM	RF and IF Characterization
Modulator characterization	

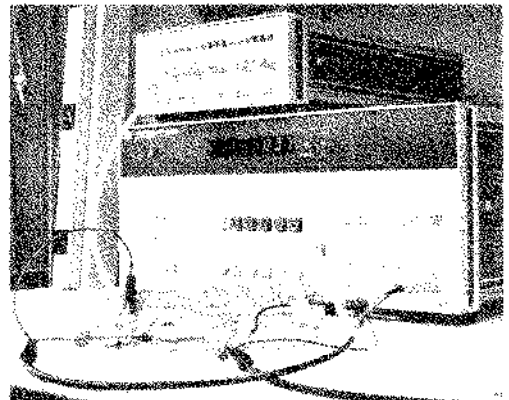

Features

Complete Signal Characterization


The 8901A Modulation Analyzer brings together in one instrument several RF signal measurement capabilities. It is more than just a high quality modulation meter. It accurately measures carrier frequency and peak input power in addition to completely characterizing modulation. This unique combination of capabilities makes the 8901A Modulation Analyzer an extremely powerful tool for analyzing signals. In normal use it eliminates the need to frequently connect and disconnect several instruments, such as counters and power meters. The Modulation Analyzer is fully programmable and can be used as part of an automatic system to make all these measurements under remote control.

FREQ: 454.52508 MHz
POWER: 43.58 mW
FM: 7.96 kHz
AM: 0.05%

Single Key Measurements

The 8901A Modulation Analyzer features easy to use controls. In automatic operation, all major functions are selected by pushing a single key. No manual tuning or range selection is needed. The Modulation Analyzer automatically tunes to the input signal, adjusts for proper signal level, selects the appropriate measurement range, makes the measurement, and displays the result.


For certain measurements manual operation may be more desirable. When selecting a specific signal in the presence of others or for special applications, the operator can easily use the Modulation Analyzer's keyboard to set any or all measurement parameters. Functions not selected manually remain in automatic mode. This greatly increases the Modulation Analyzer's versatility.

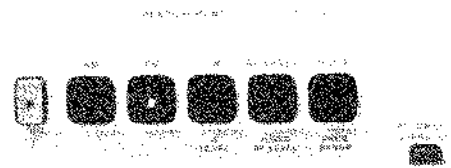

High Performance

The 8901A Modulation Analyzer offers a significant advancement in modulation measurements. Modulation depth and deviation are measured with unprecedented 1 percent accuracy. To complement this capability, optional calibrators with 0.1 percent depth or deviation accuracy can be included in the Analyzer.

A significant improvement has also been made in the area of residual noise. The extremely low internal noise of the Modulation Analyzer makes possible residual AM and FM measurements even on very stable signals. Accurate measurement of signals with small incidental AM or FM modulation are now easily performed. Residual AM in a 50 Hz to 3 kHz bandwidth is <0.02 percent, and residual FM in the same bandwidth is <8 Hz at 1300 MHz decreasing to <1 Hz below 100 MHz.

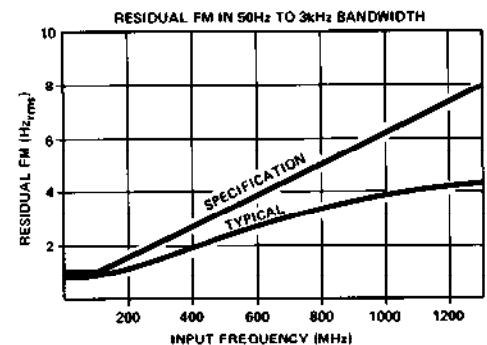


Description

The 8901A Modulation Analyzer is a complete measurement system for accurately characterizing signals in the 150 kHz to 1300 MHz frequency range. It can make more than just a single form of measurement; it combines the capabilities of three separate instruments. The 8901A Modulation Analyzer has the capability of a frequency counter for measuring carrier frequency. It can measure RF peak power with typical measurement accuracy of ± 7 dB. It can also accurately measure modulation and recover the modulating signal. This allows the user to make those measurements most commonly needed to totally characterize a signal. The Modulation Analyzer can measure a signal's frequency, frequency drift, peak power level, AM, FM, or ϕ M, and AM and FM noise components. It recovers the modulating signal with very low added distortion for audio analysis.

Besides combining several measurements in one instrument the 8901A Modulation Analyzer makes a second contribution to signal analysis—extremely precise modulation measurements. Its ability to make highly precise depth and deviation measurements coupled with very low internal noise enables the analyzer to characterize very accurate signal sources. Modulation depth or deviation accuracy is generally <1 percent of reading. Residual noise in a 50 Hz to 3 kHz bandwidth is 0.02 percent for AM and <8 Hz for FM at 1300 MHz carrier frequencies, decreasing to <1 Hz below 100 MHz.

The Modulation Analyzer is fully automatic and all major measurements can be made by pushing a single key. The Modulation Analyzer's large digital display

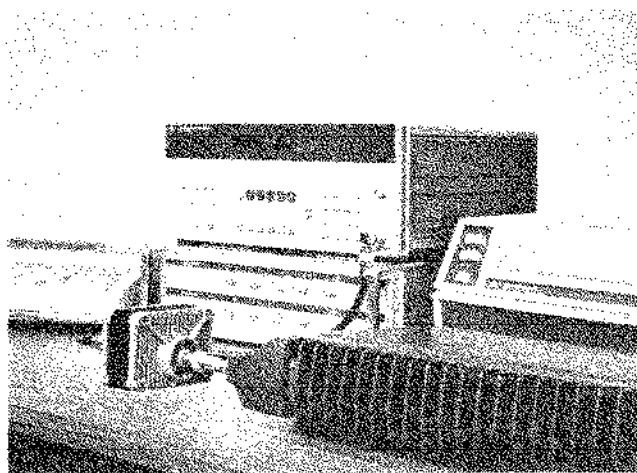

Automatic system for testing mobile transmitters.


* HP-IB is Hewlett-Packard's Implementation of IEEE Standard 488.

shows measurement results with excellent resolution and is easy to read. All measurements can be easily controlled remotely and data transferred via the Hewlett-Packard Interface Bus (HP-IB).*

FREQUENCY MEASUREMENTS. In automatic operation the 8901A Modulation Analyzer has the performance of a high quality 150 kHz to 1300 MHz frequency counter. Resolution is 10 Hz below 1000 MHz and 100 Hz above 1000 MHz. Sensitivity is -25 dBm (12 mV_{rms}) below 650 MHz and -20 dBm (22 mV_{rms}) above 650 MHz.

Besides normal frequency measurement capabilities the Analyzer's counter has several additional capabilities. Like most frequency counters it will measure signals over a wide dynamic range, >50 dB (22 mV_{rms} to 7 V_{rms}), and is protected from damage for signals up to 35 V_{rms}. Unlike many frequency counters, however, it automatically adjusts itself as the input level changes. There is no need to manually set or adjust any input attenuator. Because the Modulation Analyzer is usually used to measure modulated signals, its frequency counter accurately measures signals with significant levels of AM modulation.

The Modulation Analyzer uses an indirect technique for measuring RF frequencies. Instead of counting directly, the input signal is down-converted to an intermediate frequency (IF) using a mixer and a local oscillator (LO). By counting the frequency of both the IF and LO and calculating their difference, the Modulation Analyzer can determine the frequency of the input signal. In automatic operation the Analyzer automatically tunes to the largest input signal and measures its frequency.

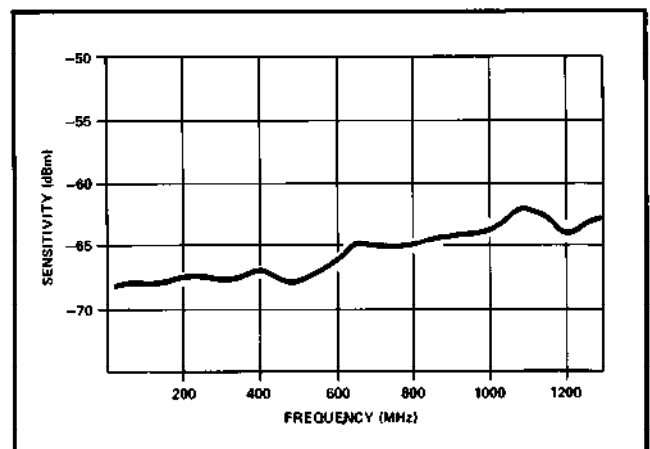


Typical sensitivity of frequency measurements in manual operation.

Description

In manual operation the user determines the frequency to which the Modulation Analyzer tunes. When more than one signal is present it is thus normally possible to select which signal is counted. Entering the approximate frequency on the keyboard causes the IF filter to eliminate all but very close interfering signals. This allows the Modulation Analyzer to selectively count signals other than the largest. Also, because of the large IF gain of the Modulation Analyzer, it is possible to measure very low-level signals. In manual operation the Modulation Analyzer has sensitivity of $0.22 \text{ mV}_{\text{rms}}$, and dynamic range of $>90 \text{ dB}$ ($0.22 \text{ mV}_{\text{rms}}$ to 7 V_{rms}).

RF POWER MEASUREMENTS. The 8901A Modulation Analyzer uses a diode detection circuit to measure RF input power. This technique measures peak voltage and is calibrated from 1 mW to 1 W for sine wave inputs. In the case of amplitude modulated signals, the Modulation Analyzer measures the peak envelope power with $\pm 1.5\text{dB}$ accuracy, thus eliminating the need for a power meter in most applications.

The Modulation Analyzer is equipped with input power protection to prevent damage from the accidental application of excessive power. This is a common cause of damage in equipment, such as the Modulation Analyzer, used to measure transmitters. The Modulation Analyzer is tested for inputs up to 25 watts. Protection is provided by limiting diodes and an RF relay. When excessive power is applied the relay opens and protects sensitive components, and the Analyzer displays an error message. The circuit automatically resets whenever a key is depressed. This technique is superior to fuses which in many cases are too slow for adequate protection and require replacement each time an overload occurs.

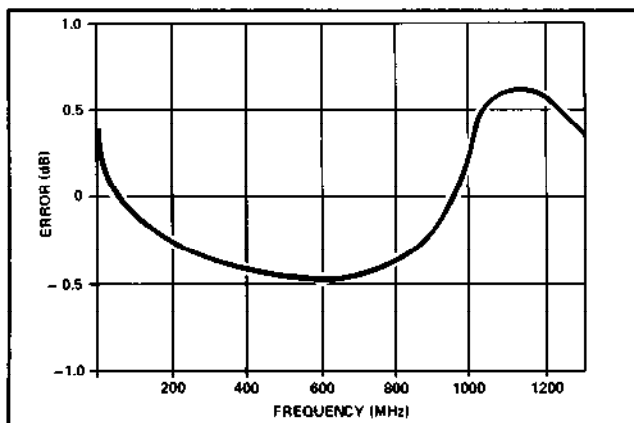

Typical power measurement accuracy.


In addition to normal RF level measurements made directly on the input signal, the Modulation Analyzer can measure the signal level in the constant-gain IF filter passband. This is the TUNED RF LEVEL function. In this mode the Analyzer accuracy is degraded from normal RF measurements, but relative power measurements at a single frequency can be made with increased resolution. Because the IF filter allows some selectivity, one signal can be measured even when others are present.

MODULATION MEASUREMENTS. In AM, high accuracy and low noise are coupled with resolution of 0.01 percent below 40 percent depth and 0.1 percent resolution to over 100 percent. AM signals at rates up to 100 kHz can be measured and the modulation accurately recovered. AM signals with significant levels of FM can be measured because of excellent FM rejection.

Most AM depth measurements can be made with accuracies better than 1 percent of reading. This is made possible by very linear amplifiers and detectors. Because these amplifiers and detectors are also low noise, residual AM in a 50 Hz to 3 kHz bandwidth is <0.02 percent rms.

FM deviation can be measured with accuracy of 1 percent and displayed with resolution ranging from 1 Hz for deviations below 4 kHz to 100 Hz for deviations greater than 40 kHz. Modulation is recovered with less than 0.1 percent distortion, and most AM is rejected.


The ability to measure low residual FM is one of the key contributions of the Modulation Analyzer. A low noise local oscillator in combination with a low noise discriminator allows residual FM measurements of $<8 \text{ Hz}$ at 1300 MHz and $<1 \text{ Hz}$ below 100 MHz. This is low enough to allow the direct measurement of residual FM of such low noise sources as crystal oscillators.

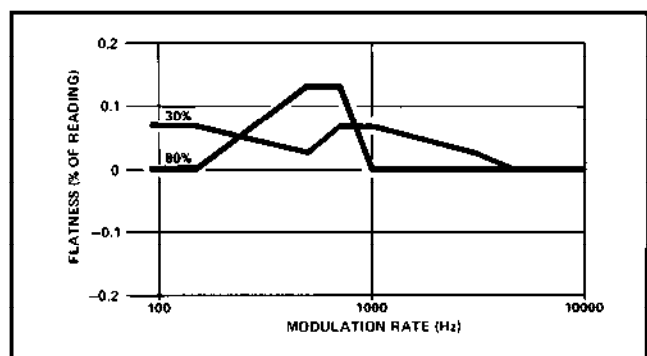


Typical AM flatness.

For all AM depth and FM deviation measurements the user can select from three detectors. Both positive and negative peak (trough for AM) can be measured. The Modulation Analyzer also has an average-responding detector which is RMS sine wave calibrated. This type of detector is useful for determining the residual noise on a signal where the RMS value and not the peak is generally the desired measurement.

The Modulation Analyzer also has a PEAK HOLD function that is used with either the positive or negative peak detectors. This function captures and displays the maximum peak modulation of a signal and is ideal for making measurements such as modulation limiting on mobile radios. PEAK HOLD can capture even very short transients and display their peak value indefinitely. Measurements can be made for any length of time and either the largest positive or negative peak that occurs will be measured. Pushing the PEAK HOLD key resets the display and initiates a new measurement cycle.

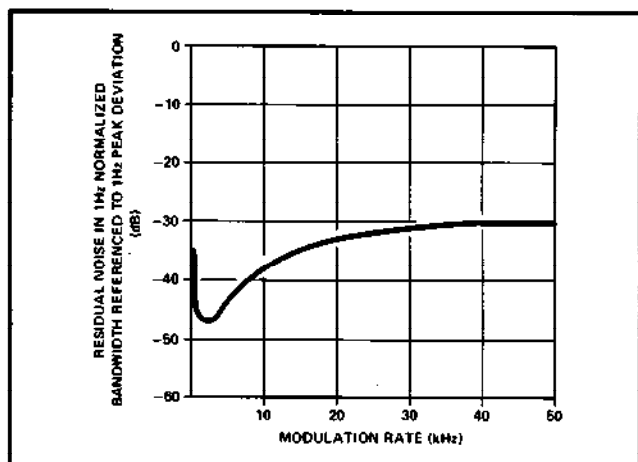

Typical internal noise contribution to FM measurements at 100 MHz carrier frequency.

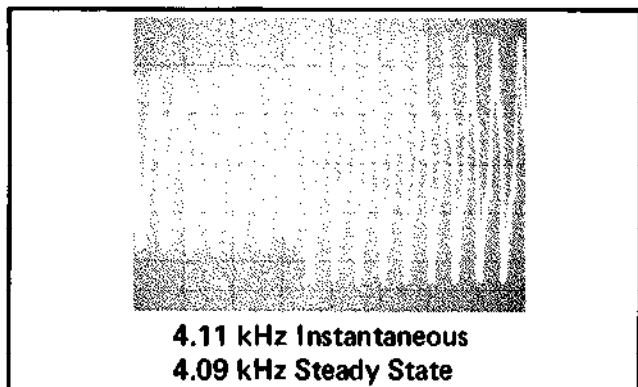


FM mobile radio modulation limiting measurement showing demodulated waveform and measured value of transient and steady-state deviation.

POST DETECTION AUDIO FILTERS. The Modulation Analyzer has two high-pass and three low-pass post-detection audio filters for filtering the recovered modulation. These filters can be selected individually or in combination. Their cutoff frequencies have been chosen to match those needed for applications such as transmitter or signal generator testing. The >20 kHz filter is a Bessel filter. It minimizes overshoot for square-wave modulation so that this type of modulating waveform can also be accurately measured.

The Modulation Analyzer contains four de-emphasis networks that can be used in addition to the audio filters. These are the ones commonly used in FM communications—25, 50, 75, and 750 μ s. When selected, the de-emphasis networks always affect the demodulated output. The user can select whether or not the de-emphasis network affects the deviation measured and indicated by the display. The ability to select either the actual or "de-emphasized deviation" increases the usefulness of the Modulation Analyzer in many applications.

MODULATION CALIBRATORS. One of the most difficult problems involved in making very accurate measurements of AM depth or FM deviation is generating a precisely modulated signal to use as a calibration standard. By ordering Option 010 a precise AM and FM modulation standard is included in the 8901A Modulation Analyzer.

The AM standard is generated by summing two identical 10 MHz signals. When one of the signals is switched on and off at a 10 kHz rate, the result is 33.33 percent AM depth. By internally measuring any slight difference in the levels of the 10 MHz signals the analyzer is able to determine the actual depth to ± 0.1 percent accuracy. To further improve the modulation envelope the rise and fall transitions are smoothed to eliminate ringing that

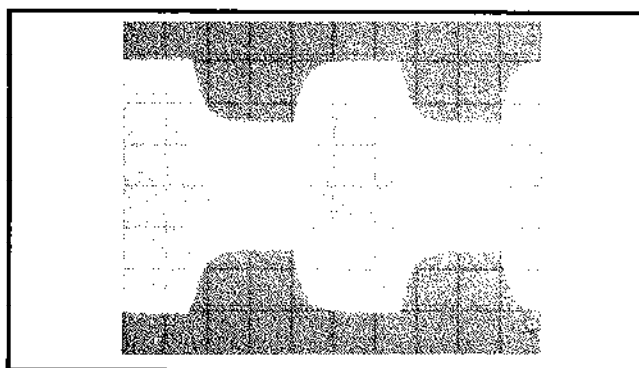

AM calibrator waveform.

Description

might otherwise occur when this signal is measured.

The FM standard is generated by square-wave modulating a VCO with a nominal 33 kHz peak deviation. By using the internal counter to measure the upper and lower frequency of this signal, the actual peak deviation is determined to ± 0.1 percent accuracy. To prevent ringing, the square wave is modified to a round edge trapezoid.


Because the modulation standards are internal to the Analyzer, there is little need for metrology laboratories to purchase separate calibration standards. Also, because of the technique used, it is easy to verify that the calibrators are operating properly.

OPERATION. Often instruments with state-of-the-art accuracy require tedious set-up or highly skilled operators in order to be used. This is not the case with the 8901A Modulation Analyzer. It provides excellent accuracy while remaining easy to use. The front panel is simple, uncluttered, and easy to understand.

The user need only select the measurement to be made. There is no need to tune, adjust levels, or select the appropriate range; the internal microprocessor does all this quickly. Because the microprocessor determines the best instrument settings, most measurements require only a single key-stroke.

For those applications requiring tuning to a specific frequency, automatic tuning may be overridden. This feature allows a single signal to be selected in the presence of others but retains the speed and convenience of the rest of the automatic functions.

The user can also make measurements relative to either a measured value or one entered from the keyboard by

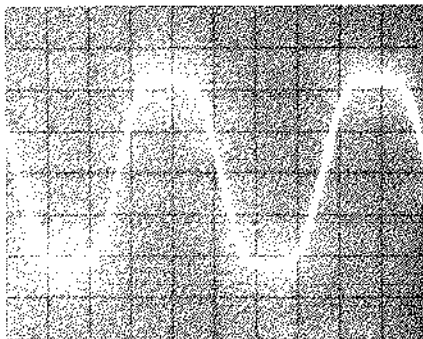

FM calibrator modulation waveform.

using the ratio keys. Relative measurements can be expressed in either dB or percent. This means that when testing FM mobile transmitters a user could enter 3 (kHz), depress the dB key, and make measurements in dB relative to 3 kHz deviation. Similarly, in broadcast FM applications, deviation could be displayed in percent relative to 75 kHz deviation where 75 kHz is defined as 100 percent. The user can also enter a measurement limit on the keyboard which will cause the Modulation Analyzer to signal whenever the measured value exceeds the value entered as a limit.

SPECIAL FUNCTIONS. The Modulation Analyzer can do more than is apparent from the front panel. This capability is accessed by using the data keys and a special function key or remotely via HP-IB. They fall into three categories: manual control of instrument functions, instrument operation verification, and service aids.

An example of the type of special function found in the manual control category is the auto tune-track mode. This mode is accessed by entering 4.1, then pressing the special key. Once the Modulation Analyzer has been placed in track mode the analyzer will continuously track the signal as it changes frequency. This eliminates the delays caused by the Analyzer searching for the signal each time the signal's frequency changes. Using this special function, a user could continuously monitor modulation accuracy on a signal generator while tuning across the signal generator's frequency band. Auto tune-track makes it possible to tune the Analyzer three ways: automatically, manually by entering the frequency on the keyboard, and track mode.

Special functions can also be used to set any measurement range or instrument function. They can be used to select either of two internal IF's, the one normally used for frequencies above 10 MHz or a narrow IF where rates and deviations are more restricted but selectivity is increased. All instrument functions not set using these special functions remain in automatic mode. This allows the user to select any combination of manual or automatic operation. By depressing the special key, the display shows an eight-digit number that indicates which functions are in automatic and the state of those manually set.

There are also numerous special functions that can be used in verifying that the instrument and its various sections are operating properly. These, along with service functions used in diagnosing and repairing the Analyzer, make repairs much faster and easier. An


additional service aid is the built-in ability to use HP signature analysis instrumentation. This allows a technician with little knowledge of digital circuits to rapidly troubleshoot a failure in the digital portion of the instrument.

Those special functions that are most commonly used in operating the Analyzer are described on the pullout information card under the front panel.

PROGRAMMABILITY. The 8901A Modulation Analyzer is completely programmable via the Hewlett-Packard Interface Bus (HP-IB). This, coupled with the ability of the Modulation Analyzer to make several measurements, the speed with which these measurements can be made, and the flexibility of the special functions, makes the Modulation Analyzer ideal for systems applications. In many instances it can reduce the number of instruments in a system, speed measurements, reduce complexity, and improve accuracy.

When the Analyzer is in remote the front panel annunciators make it very easy to determine what state the Analyzer is in.

APPLICATIONS. The 8901A Modulation Analyzer is a useful tool for analyzing many types of signals. Often it can provide needed information that has been difficult to obtain such as incidental FM or residual FM. It can replace large, complex test systems, and speed and simplify measurements.

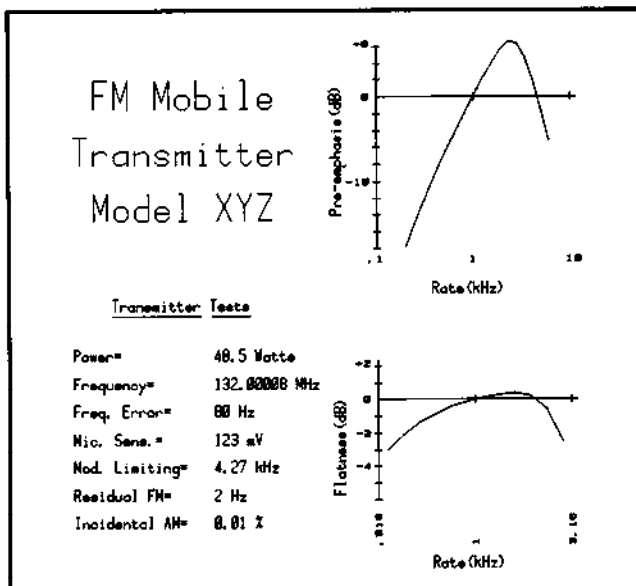


Output of mobile radio automatic test.

The Modulation Analyzer is superbly capable of measuring transmitters used in mobile communications. This single instrument can be used in making most of the measurements made on transmitters.

The Modulation Analyzer can be equally useful for other types of transmitters. For avionics applications it can be very useful in measuring navigation signals. In testing ILS transmitters the Analyzer can be used to very accurately measure depth of modulation. For broadcast AM and FM it can be used to measure AM depth or FM deviation, and it can accurately recover the modulation for making measurements such as stereo separation.

With its accuracy the Modulation Analyzer makes an excellent addition to a metrology laboratory. An example of its usefulness is in calibrating signal generators, especially high performance signal generators such as the HP 8640B. The Modulation Analyzer's capabilities exceed those required to verify many signal generator specifications. Besides improving the accuracy of these measurements it greatly reduces the time involved in making measurements. Also, the optional calibrators provide a new level of modulation standard accuracy and help ensure accurate measurements. They also enhance the calibration of the Modulation Analyzer itself.

Because the Modulation Analyzer is useful for characterizing all types of signals in general, it is very useful in research and development laboratories. It can be used for characterizing VCO's, measuring residual noise on crystal oscillators, measuring incidental modulation, measuring frequency on low level signals, etc. When used with a signal source it can be used to characterize RF and IF designs, evaluate modulators, and test individual IC's or modules.

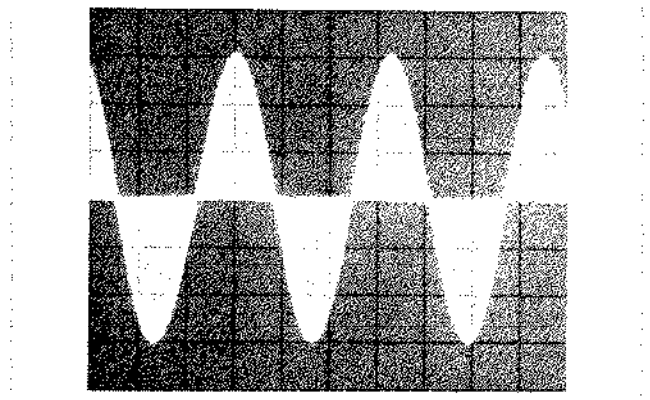

Demodulated FM stereo test signal at 15 kHz rate.

8901A Specifications

All parameters describe performance in automatic operation or properly set manual conditions. SPECIFICATIONS describe the instrument's warranted performance. SUPPLEMENTAL CHARACTERISTICS (shown in italics) are intended to provide information useful in applying the instrument by giving typical, but non-warranted, performance parameters.

RF INPUT

Frequency Range: 150 kHz to 1300 MHz.

Operating Level:

150 kHz - 650 MHz: 12 mV_{rms} (-25 dBm) to 7 V_{rms} (1 W_{peak}).

650 MHz - 1300 MHz: 22 mV_{rms} (-20 dBm) to 7 V_{rms} (1 W_{peak}).

Supplemental Characteristics:

Tuning: Automatic, track (frequencies >10 MHz), manual frequency entry

Acquisition Time (Automatic Operation): ~1.5 second.

Input Impedance: 50Ω nominal.

Maximum Safe Input Level:

AC: 35 V_{rms} (25 W for source SWR <4).

DC: 40 V.

FREQUENCY MODULATION

Rates: 150 kHz - 10 MHz: 20 Hz to 10 kHz.

10 MHz - 1300 MHz: 20 Hz to 200 kHz.¹

Deviations:

150 kHz - 10 MHz: 40 kHz_{peak} maximum.

10 MHz - 1300 MHz: 400 kHz_{peak} maximum.¹

Accuracy:²

250 kHz - 10 MHz: ±2% of reading ±1 digit, 20 Hz to 10 kHz rates.

10 MHz - 1300 MHz: ±1% of reading ±1 digit, 50 Hz to 100 kHz rates.

±5% of reading ±1 digit, 20 Hz to 200 kHz rates.

Demodulated Output Distortion:³

400 kHz - 10 MHz: <0.1% THD, deviations <10 kHz.

10 MHz - 1300 MHz: <0.1% THD, rates and deviations <100 kHz.

AM Rejection (for 50% AM at 400 Hz and 1 kHz rates):² <20 Hz peak deviation measured in a 50 Hz to 3 kHz BW.

Residual FM (50 Hz to 3 kHz BW): <8 Hz_{rms} at 1300 MHz, decreasing linearly with frequency to <1 Hz_{rms} for 100 MHz and below.

Supplemental Characteristics:

Maximum Deviation Resolution:

1 Hz, <4 kHz deviation.

10 Hz, 4 kHz to 40 kHz deviation.

100 Hz, 40 kHz to 400 kHz deviation.

Resolution is increased one digit with 750 μs de-emphasis and pre-display "on."

Demodulated Output Distortion: 150 to 400 kHz; <0.3% THD, deviations <10 kHz

Detectors: + peak, - peak, and average (rms sine wave calibrated).

Demodulated Output across an Open circuit (600Ω output impedance):⁴

1 mV/Hz when resolution is 1 Hz.

0.1 mV/Hz when resolution is 10 Hz.

0.01 mV/Hz when resolution is 100 Hz.


Stereo Separation (50 Hz to 15 kHz): >47 dB.

PHASE MODULATION

Carrier Frequency: 10 MHz to 1300 MHz.

Rates: 200 Hz to 20 kHz.

Deviation and Maximum Resolution:

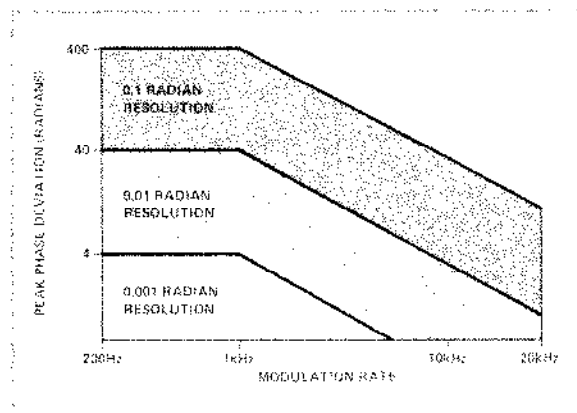

Accuracy:² ±3% of reading ±1 digit.

Demodulated Output Distortion: <0.1% THD.

AM Rejection (for 50% AM at 1 kHz rates):² <0.03 radians, peak deviation.

Supplemental Characteristics:

Modulation Rates: Usable from 20 Hz to 100 kHz with degraded performance.

Detectors: + peak, - peak, average (rms sine wave calibrated).

Demodulated Output across an Open Circuit (600Ω output impedance):⁴

1 V/rad when resolution is 0.001 radian.

0.1 V/rad when resolution is 0.01 radian.

0.01 V/rad when resolution is 0.1 radian.

AMPLITUDE MODULATION

Rates: 150 kHz - 10 MHz: 20 Hz to 10 kHz.

10 MHz - 1300 MHz: 20 Hz to 100 kHz.

Depth: to 99%.

¹ Maximum rate 20 kHz and peak deviation 40 kHz with 750 μs de-emphasis filter.

² Peak residuals must be accounted for in peak readings.

³ With 750 μs de-emphasis and pre-display "off," distortion is not specified for modulation outputs >4 V peak. This can occur near maximum deviation for a measurement range at rates <2 kHz.

⁴ For optimum flatness, cables should be terminated with their characteristic impedance.

Accuracy:^{2,8}

150 kHz to 10 MHz: $\pm 2\%$ of reading ± 1 digit,
50 Hz to 10 kHz rates, $> 5\%$ depth.
 $\pm 3\%$ of reading ± 1 digit, 20 Hz to 10 kHz rates.
10 MHz to 1300 MHz: $\pm 1\%$ of reading ± 1 digit,
50 Hz to 50 kHz rates, $> 5\%$ depth.
 $\pm 3\%$ of reading ± 1 digit, 20 Hz to 100 kHz rates.

Flatness (Variation in indicated AM depth for constant depth on input signal):

10 MHz to 1300 MHz: $\pm 0.3\%$ of reading ± 1 digit,
90 Hz to 10 kHz rates, 20 to 80% depth.

Demodulated Output Distortion: $< 0.3\%$ THD for $\leq 50\%$ depth, $< 0.6\%$ THD for $\leq 95\%$ depth.**FM Rejection (at 400 Hz and 1 kHz rates, 50 Hz to 3 kHz BW):**²

250 kHz to 10 MHz: $< 0.2\%$ AM for < 5 kHz_{peak} deviation.
10 MHz to 1300 MHz: $< 0.2\%$ AM for < 50 kHz_{peak} deviation.

Residual AM (50 Hz to 3 kHz BW): $< 0.01\%$ _{rms}.**Supplemental Characteristics:****Maximum Depth Resolution:**

0.01% for depths $\leq 39.99\%$.
0.1% for depths $\geq 40\%$.

Detectors: peak [+ peak], trough [- peak], average (rms sine wave calibrated).

Demodulated Output across an Open Circuit (600 Ω output impedance):⁴

0.1 V/percent when resolution is 0.01%.
0.01 V/percent when resolution is 0.1%.

FREQUENCY COUNTER

Range: 150 kHz - 1300 MHz.

Sensitivity:

150 kHz - 650 MHz: 12 mV_{rms} (-25 dBm).
650 MHz - 1300 MHz: 22 mV_{rms} (-20 dBm).

Accuracy: Reference accuracy ± 3 counts of least significant digit.

Internal Reference:

Frequency: 10 MHz.

Aging rate: $< 1 \times 10^{-6}$ /month
(Optional: $< 1 \times 10^{-9}$ /day)⁵.

Supplemental Characteristics:

Modes: Frequency, and Frequency Error (displays the difference between the frequency entered via the keyboard and the actual RF input frequency).

Sensitivity in manual tuning mode: Approximate frequency must be entered from keyboard. 0.22 mV_{rms} (-60 dBm).

Maximum Resolution: 10 Hz for frequencies < 1 GHz.
100 Hz for frequencies ≥ 1 GHz.

Internal Reference Accuracy: Overall accuracy is a function of time base calibration \pm aging rate \pm temperature effects \pm line voltage effects \pm short term stability.

	Standard	Option 002
Aging Rate	$< 1 \times 10^{-6}$ /mo.	$< 1 \times 10^{-9}$ /day
Temperature Effects	$< 2 \times 10^{-7}$ /°C	$< 2 \times 10^{-10}$ /°C
Line Voltage Effects (+5%, -10% line voltage change)	$< 1 \times 10^{-6}$	$< 6 \times 10^{-10}$
Short term stability	—	$< 1 \times 10^{-3}$ for 1s average

RF LEVEL

(Peak voltage responding, rms sine wave power calibrated).

Range: 1 mW to 1 W.

Accuracy: ± 1.5 dB

SWR: ≤ 650 MHz: < 1.3 in a 50 Ω system.
 < 1300 MHz: < 1.5 in a 50 Ω system.

Supplemental Characteristics:

Typical Accuracy: 150 kHz-650 MHz: ± 0.5 dB
650 MHz-1300 MHz: ± 1.0 dB

Resolution: 0.1 mW for levels 0.1 to 1 W.

0.01 mW for levels 0.01 to 0.1 W.

0.001 mW for levels < 0.01 W.

AUDIO FILTERS

High pass (3 dB cutoff frequency): 50 Hz and 300 Hz.

Low pass (3 dB cutoff frequency except > 20 kHz filter): 3 kHz, 15 kHz, > 20 kHz.

De-emphasis filters: 25 μ s, 50 μ s, 75 μ s, and 750 μ s.
De-emphasis filters are single pole low pass filters whose 3 dB frequencies are 6366 Hz for 25 μ s, 3183 Hz for 50 μ s, 2122 Hz for 75 μ s, and 212 Hz for 750 μ s.

Flatness:

50 Hz High Pass: $< 1\%$ at rates ≥ 200 Hz.
300 Hz High Pass: $< 1\%$ at rates ≥ 1 kHz.
3 kHz Low Pass: $< 1\%$ at rates ≤ 1 kHz.
15 kHz Low Pass: $< 1\%$ at rates ≤ 10 kHz.
 > 20 kHz Low Pass: $< 1\%$ at rates ≤ 10 kHz.

Supplemental Characteristics:

50 Hz and 300 Hz High Pass: Two pole.

3 kHz and 15 kHz Low Pass: Five pole.

> 20 kHz Low Pass: Nine pole Bessel (typically 3 dB at 100 kHz).

High and Low Pass 3 dB Frequency Accuracy: $\pm 3\%$.

De-emphasis Filter Time Constant Accuracy: $\pm 3\%$.

Overshoot on square wave modulation (> 20 kHz Low Pass Filter⁴): $< 1\%$.

² Peak residuals must be accounted for in peak readings.

⁴ For optimum flatness, cables should be terminated with their characteristic impedance.

⁵ After 30-day warm-up.

⁶ The > 20 kHz low pass filter is intended for minimum overshoot with square wave modulation.

⁷ External reference accuracy affects accuracy of all measurements.

⁸ For peak measurements only, AM accuracy may be affected by distortion generated by the Modulation Analyzer. In the worst case this can decrease accuracy by 0.1% of reading for each 0.1% of distortion.

8901A Specifications

All parameters describe performance in automatic operation or properly set manual conditions. SPECIFICATIONS describe the instrument's warranted performance. SUPPLEMENTAL CHARACTERISTICS (shown in italics) are intended to provide information useful in applying the instrument by giving typical, but non-warranted, performance parameters.

REAR PANEL INPUTS/OUTPUTS

Supplemental Characteristics:

FM Output: 10 k Ω impedance, -9 V to 6 V into an open circuit; ~6 V/MHz, dc coupled, 16 kHz bandwidth (one pole).

AM Output: 10 k Ω impedance, -4 V to 0 V into an open circuit, ~8 mV/%, dc coupled, 16 kHz bandwidth (one pole).

Recorder Output: DC voltage proportional to peak voltage of the MODULATION OUTPUT, 1 k Ω impedance, 0 V to 4 V for each resolution range into an open circuit.

IF Output: 50 Ω impedance, 150 kHz to 2.5 MHz, -27 dBm to -3 dBm.

10 MHz Reference Output: 50 Ω impedance, TTL levels (0 V to >2.2 V into an open circuit), available only with Option 002 1x10⁻⁹/day internal reference, outputs internal reference only.

10 MHz Reference Input:² >500 Ω impedance, 0.5 V_{peak-to-peak} minimum input level.

LO Input (Option 003): 50 Ω impedance, ~1.27 MHz to 1301.5 MHz, 0 dBm.

CALBRATORS (Option 010)

AM Calibrator Depth and Accuracy: 33.33% depth nominal, internally calibrated to an accuracy of $\pm 0.1\%$.

FM Calibration Deviation and Accuracy: 34 kHz_{peak} deviation nominal, internally calibrated to an accuracy of $\pm 0.1\%$.

Supplemental Characteristics:

Carrier Frequency: 10.1 MHz.

Modulation Rate: 10 kHz.

Output Level: -25 dBm.

GENERAL

Temperature: Operating 0° to 55°C.

Storage: -55°C to 75°C.

Remote Operation: HP-IB; all functions except the line switch are remotely controllable.

HP-IB compatibility; as defined in IEEE 488-1978 is: SH1, AH1, T5, TE0, L3, LE0, SR1, RL1, PP0, DC1, DT1, C0


EMI: Conducted and radiated interference is within the requirements of methods CE03 and RE02 of MIL STD 461A (for inputs <10 mW), VDE 0871 (Level B), and CISPR publication 11.

Conducted and Radiated Susceptibility: Meets the requirements of methods CS01, CS02, and RS03 (1 volt/meter) of MIL STD 461A dated 1968.

Power: 100, 120, 220, or 240 V (+5, -10%); 48-66 Hz; 200 VA max.

Weight: Net 20 kg (44 lb); shipping 25 kg (55 lb).

Dimensions: 190 mm H x 425 mm W x 468 mm D (7.5 in. x 16.8 in. x 18.4 in.).

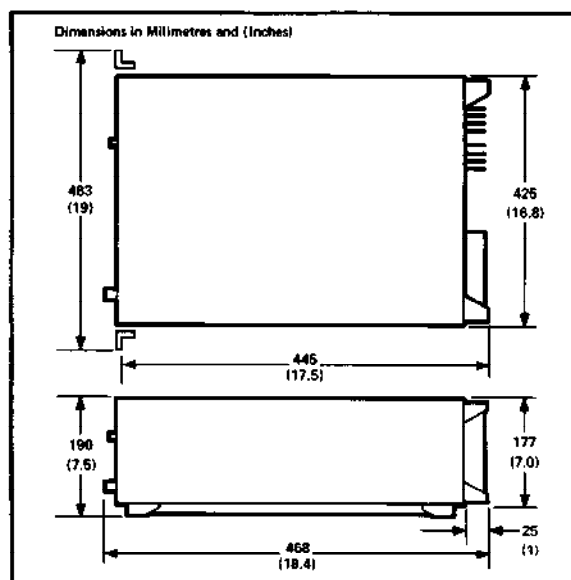

MODEL NUMBER AND NAME

8901A Modulation Analyzer

Option 001: Rear panel instead of front panel connections for input, modulation output, calibrators.

Option 002: 1x10⁻⁹/day internal reference oscillator.

Option 003: Rear panel connections which allow use with an external local oscillator

Option 004: Operation from 48 to 440 Hz power line

Option 010: AM and FM calibrators

Option 907: Front panel handle kit

Option 908: Rack mounting flange kit

Option 909: Front panel handle plus rack mounting flange kit

Option 910: Extra manual

For more information, call your local HP Sales Office or nearest Regional Office: • Eastern (301) 258-2000; • Midwestern (312) 255-9800; • Southern (404) 955-1500; • Western (213) 506-3700; • Canadian (416) 678-9430. Ask the operator for instrument sales. Or write Hewlett-Packard, 1820 Embarcadero Rd., Palo Alto, CA 94303. In Europe: Hewlett-Packard S.A., 7, Rue du Bois-du-Lan, P.O. Box CH 1217 Meyrin 2, Geneva, Switzerland. In Japan: Yokogawa-Hewlett-Packard Ltd., 29-21, Takaido-Higashi 3-chome, Suganami-ku, Tokyo 168.

Printed in U.S.A.