

**E5505A  
Phase Noise  
Measurement System**

**for E5500 Software Rev A.03.00**

**SCPI Command Reference**  
**First edition, June 2004**



**Agilent Technologies**

# Notices

© Agilent Technologies, Inc. 2004

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Agilent Technologies, Inc. as governed by United States and international copyright laws.

Windows® and MS Windows® are U.S. registered trademarks of Microsoft Corporation.

## Manual Part Number

E5505-90002

## Edition

First edition, June 2004

Printed in USA

Agilent Technologies, Inc.  
1400 Fountaingrove Pkwy  
Santa Rosa, CA 95403

## Warranty

The material contained in this document is provided "as is," and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

## Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

## Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as "Commercial computer software" as defined in DFAR 252.227-7014 (June 1995), or as a "commercial item" as defined in FAR 2.101(a) or as "Restricted computer software" as defined in FAR 52.227-19 (June 1987) or any equivalent

agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies' standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

## Safety Notices

### CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

### WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

# Contents

## 1 SCPI Interface

Introduction	38
Configuring the SCPI Interface	39
Configuring Telnet and sockets interfaces	39
Configuring the RS-232 interface	39
Configuring the VXI-11 interface	39
Figure 1. E5500 block diagram	40
Figure 2. E5500 navigate to I_O Config	41
Figure 3. Select internal instrument	41
Figure 4. Accept default settings	42
Figure 5. Configured default settings	42
Figure 6. Navigate to LAN server	43
Starting the SCPI Interface	44
Figure 7. Navigate to SCPI interface	44
Figure 8. Choosing the interface	45
Figure 9. SCPI interface information	45
SCPI logging function	46
Figure 10. E5500 LAN client logging	46
Starting the SCPI Interface Programmatically	47
DOS command prompt example	47

## 2 SCPI Assistant

Starting the SCPI Assistant	50
Figure 11. Navigate to SCPI assistant	50
Figure 12. SCPI assistant interface	51
SCPI logging function	51
Figure 13. E5500 LAN client logging	51

## 3 SCPI Program Examples

Application Environment Setup	54
HTBasic for Windows on same PC or remote PC	54
RMBUX on remote workstation	54
Agilent Vee on same PC or remote PC	55
Figure 14. Add IP address	55
SCPI Programming	56
Set up the measurement definition	56
Read the data from the measurement	57
HTBasic for Windows Program Example	58

## 4 E5500 SCPI Commands

Syntax Conventions	64
Table 1. Notation conventions and definitions	64
Status Registers	65
Figure 15. Event status register 1	66
Figure 16. Event status register 2	67
Full Command List	68
Format of measurement data output	68
SCPI commands	68
CALCulate	69
CALibrate	70
FORMAT	71
INITiate	71
MMEMory	71
PAUSE	71
SOURce	73
STATus	74
SYSTem	74

## 5 Required Commands

Required Commands Introduction	78
*CLS	79
Command syntax	79
Query syntax	79
Attribute summary	79
Additional information	79
*ESE	80
Command syntax	80
Example	80
Query syntax	80
Attribute summary	80
Additional information	80
*ESR?	81
Command syntax	81
Query syntax	81
Return format	81
Attribute summary	81
Additional information	81
*IDN?	82
Command syntax	82

Example	82
Query syntax	82
Return format	82
Attribute summary	82
*OPC	83
Command syntax	83
Query syntax	83
Return format	83
Attribute summary	83
Additional information	83
*OPC?	84
Command Syntax	84
Query syntax	84
Return format	84
Attribute summary	84
Additional information	84
*RST	85
Command syntax	85
Query syntax	85
Attribute summary	85
Additional information	85
*SRE	89
Command syntax	89
Example	89
Query syntax	89
Return format	89
Attribute summary	89
Additional information	89
*STB?	90
Command syntax	90
Query syntax	90
Return format	90
Attribute summary	90
Additional information	90
*TST?	91
Command syntax	91
Query syntax	91
Return format	91
Attribute summary	91
Additional information	91
*WAI	92

Command syntax	92
Query syntax	92
Attribute summary	92
Additional information	92

## 6 ABORt Commands

ABORt	94
Command syntax	94
Example	94
Query syntax	94
Attribute summary	94

## 7 CALCulate Commands

CALCulate Commands Introduction	97
CALCulate:ACCumulated[PHASE]?	99
Command Syntax	99
Query syntax	99
Example	99
Return format	99
Attribute summary	99
Additional information	99
CALCulate:AVARiance?	100
Command Syntax	100
Query syntax	100
Example	100
Return format	100
Attribute summary	100
Additional information	100
CALCulate:CFSCale	101
Command syntax	101
Example	101
Query syntax	101
Return format	101
Attribute summary	101
Additional information	101
CALCulate:DATA?	102
Command syntax	102
Query syntax	102
Return format	102
Attribute summary	102
Additional information	102

CALCulate:DATA:HEADER:POINTs?	104
Command Syntax	104
Query syntax	104
Example	104
Return format	104
Attribute summary	104
CALCulate:DIPower	105
Command syntax	105
Example	105
Query syntax	105
Return format	105
Attribute summary	105
Additional information	105
CALCulate:F20Scillator[:COMPARE]	106
Example	106
Query syntax	106
Attribute summary	106
Additional information	106
CALCulate:F30Scillator[:COMPARE]	108
Command syntax	108
Example	108
Query syntax	108
Attribute summary	108
Additional information	108
CALCulate:INTegral?	110
Command Syntax	110
Query syntax	110
Example	110
Return format	110
Attribute summary	110
Additional information	110
CALCulate:INTegral:TYPE	111
Command Syntax	111
Example	111
Query syntax	111
Return format	111
Attribute summary	111
Additional information	111
CALCulate:LIMit:NOISe:MAXimum	112
Example	112
Query syntax	112

Return format	112
Attribute summary	112
Additional information	112
CALCulate:LIMit:NOISe:MAXimum:DELete	113
Command syntax	113
Example	113
Query syntax	113
Attribute summary	113
CALCulate:LIMit:NOISe:MAXimum: DELete:ALL	114
Command syntax	114
Example	114
Query syntax	114
Attribute summary	114
CALCulate:LIMit:NOISe:MAXimum:DISPlay	115
Command syntax	115
Example	115
Query syntax	115
Return format	115
Attribute summary	115
CALCulate:LIMit:NOISe:MAXimum:FAIL?	116
Command Syntax	116
Example	116
Query syntax	116
Return format	116
Attribute summary	116
Additional information	116
CALCulate:LIMit:NOISe:MAXimum:FAIL: ALL?	117
Command Syntax	117
Example	117
Query syntax	117
Return format	117
Attribute summary	117
Additional information	117
CALCulate:LIMit:NOISe:MINimum	118
Command syntax	118
Example	118
Query syntax	118
Return format	118
Attribute summary	118

Additional information	118
CALCulate:LIMit:NOISe:MINimum:DELete	119
Command syntax	119
Example	119
Query syntax	119
Attribute summary	119
CALCulate:LIMit:NOISe:MINimum: DELete:ALL	120
Command syntax	120
Example	120
Query syntax	120
Attribute summary	120
CALCulate:LIMit:NOISe:MINimum:DISPlay	121
Command syntax	121
Example	121
Query syntax	121
Return format	121
Attribute summary	121
CALCulate:LIMit:NOISe:MINimum:FAIL?	122
Command Syntax	122
Example	122
Query syntax	122
Return format	122
Attribute summary	122
Additional information	122
CALCulate:LIMit:NOISe:MINimum: FAIL:ALL?	123
Command Syntax	123
Example	123
Query syntax	123
Return format	123
Attribute summary	123
Additional information	123
CALCulate:LIMit:SPUR:MAXimum	124
Command syntax	124
Example	124
Query syntax	124
Return format	124
Attribute summary	124
Additional information	124
CALCulate:LIMit:SPUR:MAXimum:DELete	125

Command syntax	125
Example	125
Query syntax	125
Attribute summary	125
CALCulate:LIMit:SPUR:MAXimum:	
DELete:ALL	126
Command syntax	126
Example	126
Query syntax	126
Attribute summary	126
CALCulate:LIMit:SPUR:MAXimum:DISPlay	127
Command syntax	127
Example	127
Query syntax	127
Return format	127
Attribute summary	127
CALCulate:LIMit:SPUR:MAXimum:FAIL?	128
Command Syntax	128
Example	128
Query syntax	128
Return format	128
Attribute summary	128
Additional information	128
CALCulate:LIMit:SPUR:MAXimum:	
FAIL:ALL?	129
Command Syntax	129
Example	129
Query syntax	129
Return format	129
Attribute summary	129
Additional information	129
CALCulate:LIMit:SPUR:MINimum	130
Command syntax	130
Example	130
Query syntax	130
Return format	130
Attribute summary	130
CALCulate:LIMit:SPUR:MINimum:DELete	131
Command syntax	131
Example	131
Query syntax	131

Attribute summary	131
CALCulate:LIMit:SPUR:MINimum:	
DELETED:ALL	132
Command syntax	132
Example	132
Query syntax	132
Attribute summary	132
CALCulate:LIMit:NOISE:MINimum:DISPlay	133
Command syntax	133
Example	133
Query syntax	133
Return format	133
Attribute summary	133
CALCulate:LIMit:SPUR:MINimum:FAIL?	134
Command Syntax	134
Example	134
Query syntax	134
Return format	134
Attribute summary	134
Additional information	134
CALCulate:LIMit:SPUR:MINimum:	
FAIL:ALL?	135
Command Syntax	135
Example	135
Query syntax	135
Return format	135
Attribute summary	135
Additional information	135
CALCulate:PBWidth	136
Command syntax	136
Query syntax	136
Example	136
Return format	136
Attribute summary	136
Additional information	136
CALCulate:SElect	137
Command syntax	137
Example	137
Query syntax	137
Return format	137
Attribute summary	137

Additional information	137
CALCulate:SMOOthing	138
Command syntax	138
Example	138
Query syntax	138
Return format	138
Attribute summary	138
Additional information	138
Command syntax	139
Example	139
Query syntax	139
Return format	139
Attribute summary	139
CALCulate:TVAReance?	140
Command Syntax	140
Query syntax	140
Return format	140
Attribute summary	140
Additional information	140
CALCulate:VIEW:SPURtable	141
Command syntax	141
Example	141
Query syntax	141
Attribute summary	141
Additional information	141
CALCulate:VIEW:TRACe	142
Command syntax	142
Query syntax	142
Return format	142
Attribute summary	142
Additional information	142
CALCulate:VIEW:XYData	143
Command syntax	143
Example	143
Query syntax	143
Attribute summary	143
Additional information	143
CALCulate:YShift	144
Command syntax	144
Example	144
Query syntax	144

Return format	144
Attribute summary	144
Additional information	144

## 8 CALibrate Commands

CALibrate Commands Introduction	146
CALibrate:DETector:CONSTant	147
Command syntax	147
Example	147
Query syntax	147
Return format	147
Attribute summary	147
Additional information	147
CALibrate:DETector:CONSTant:METHod	148
Command syntax	148
Example	148
Query syntax	148
Return format	148
Attribute summary	148
Additional information	148
CALibrate:DETector:CONSTant:SPUR:	
AMPLitude	150
Command syntax	150
Example	150
Query syntax	150
Return format	150
Attribute summary	150
CALibrate:DETector:CONSTant:SPUR:OFFSet	151
Command syntax	151
Example	151
Query syntax	151
Return format	151
Attribute summary	151
CALibrate:VCO:IRESistance	152
Command syntax	152
Example	152
Query syntax	152
Return format	152
Attribute summary	152
Additional information	152
CALibrate:VCO:PLLSuppress	153

Command syntax	153
Example	153
Query syntax	153
Return format	153
Attribute summary	153
Additional information	153
CALibrate:VCO:PLLSuppress:APOLe?	155
Query syntax	155
Return format	155
Attribute summary	155
Additional information	155
CALibrate:VCO:PLLSuppress:CBWidth?	156
Query syntax	156
Return format	156
Attribute summary	156
Additional information	156
CALibrate:VCO:PLLSuppress:DISPlay	
[:ALWays]	157
Command syntax	157
Example	157
Query syntax	157
Return format	157
Attribute summary	157
CALibrate:VCO:PLLSuppress:ERRor	158
Command syntax	158
Example	158
Query syntax	158
Return format	158
Attribute summary	158
CALibrate:VCO:PLLSuppress:ERRor:ACTion	159
Command syntax	159
Example	159
Query syntax	159
Return format	159
Attribute summary	159
Additional information	159
CALibrate:VCO:PLLSuppress:PTRange?	160
Query syntax	160
Return format	160
Attribute summary	160
Additional information	160

CALibrate:VCO:TCONstant?	161
Command Syntax	161
Query syntax	161
Return format	161
Attribute summary	161
Additional information	161
CALibrate:VCO:TCONstant:METHod	162
Command syntax	162
Example	162
Query syntax	162
Return format	162
Attribute summary	162
Additional information	162
CALibrate:VCO:TCONstant:NOMinal	164
Command syntax	164
Example	164
Query syntax	164
Return format	164
Attribute summary	164
Additional information	164
CALibrate:VCO:TMODE	165
Command syntax	165
Example	165
Query syntax	165
Return format	165
Attribute summary	165
Additional information	165
CALibrate:VCO:VCADjust	166
Command syntax	166
Example	166
Query syntax	166
Return format	166
Attribute summary	166
CALibrate:VCO:VCENTER	167
Command syntax	167
Example	167
Query syntax	167
Return format	167
Attribute summary	167
Additional information	167
Table 2. Voltage Tune Range	167

CALibrate:VCO:VRANge	168
Command syntax	168
Example	168
Query syntax	168
Return format	168
Attribute summary	168
Additional information	168

## 9 DISPLAY Commands

DISPlay Commands Introduction	170
DISPlay:GRAPh:BOUNds:AMPLitude	171
Command syntax	171
Command Example	171
Query syntax	171
Query Example	171
Return format	171
DISPlay:GRAPh:BOUNds:AMPLitude?	173
Command Syntax	173
Query syntax	173
Example	173
Return format	173
Attribute summary	173
DISPlay:GRAPh:BOUNds:FREQuency	174
Command syntax	174
Example	174
Query syntax	174
Return format	174
Attribute summary	174
DISPlay:GRAPh:CFSCale	175
Command syntax	175
Example	175
Query syntax	175
Return format	175
Attribute summary	175
Additional information	175
DISPlay:GRAPh:DIPower	176
Command syntax	176
Example	176
Query syntax	176
Return format	176
Attribute summary	176

DISPlay:GRAPh:PBWidth	177
Command syntax	177
Example	177
Query syntax	177
Return format	177
Attribute summary	177
Additional information	177
DISPlay:GRAPh:SMOothing	178
Command syntax	178
Example	178
Query syntax	178
Return format	178
Attribute summary	178
Additional information	178
DISPlay:GRAPh:TRANSform	179
Command syntax	179
Example	179
Query syntax	179
Return format	179
Attribute summary	179
Additional information	179
DISPlay:GRAPh:YShift	180
Command syntax	180
Example	180
Query syntax	180
Return format	180
Attribute summary	180
DISPlay:MEASurement:TIME?	181
Query syntax	181
Return format	181
Attribute summary	181
Additional information	181
DISPlay:TEXT:TITLe	182
Command syntax	182
Query syntax	182
Example	182
Return format	182
Attribute summary	182

## 10 FORMat Commands

FORMat Command Introduction	184
-----------------------------	-----

FORMat[:DATA]	185
Command Syntax	185
Example	185
Query syntax	185
Return format	185
Attribute summary	185
Additional information	185

## 11 INITiate Commands

INITiate Commands Introduction	188
INITiate[:IMMEDIATE][:ALL]	189
Command syntax	189
Example	189
Query syntax	189
Attribute summary	189
INITiate[:IMMEDIATE]:CALibrate	190
Command syntax	190
Example	190
Query syntax	190
Attribute summary	190
Additional information	190
INITiate[:IMMEDIATE]:MEASure	191
Command syntax	191
Example	191
Query syntax	191
Attribute summary	191

## 12 MMEMory Commands

MMEMory:LOAD[:ALL]	195
Command syntax	195
Example	195
Attribute summary	195
Additional information	195
MMEMory:STORe	196
Command syntax	196
Example	196
Query syntax	196
Return format	196
Attribute summary	196
Additional information	196

## 13 PAUSE Commands

PAUSE Commands Introduction	198
PAUSE:ABORT:AUTO	199
Command syntax	199
Example	199
Query syntax	199
Return format	199
Attribute summary	199
Additional information	199
PAUSE:ADJust:LNAGain	200
Command syntax	200
Example	200
Query syntax	200
Return format	200
Attribute summary	200
Additional information	200
PAUSE:ADJust:VCOCenter	201
Command syntax	201
Example	201
Query syntax	201
Return format	201
Attribute summary	201
Additional information	201
PAUSE:CONNect	202
Command syntax	202
Example	202
Query syntax	202
Return format	202
Attribute summary	202
Additional information	202
PAUSE:CONTinue	203
Command syntax	203
Example	203
Query syntax	203
Attribute summary	203
PAUSE:RETRy	204
Command syntax	204
Query syntax	204
Example	204
Attribute summary	204

PAUSE:SPECial	205
Command syntax	205
Query syntax	205
Example	205
Return format	205
Attribute summary	205

## 14 SENSe Commands

SENSe Commands Introduction	209
-----------------------------	-----

[SENSe:]DATA?	211
Command Syntax	211
Query syntax	211
Return format	211
Attribute summary	211
Additional information	211

[SENSe:]DATA:HEADER:POINTS?	212
Command Syntax	212
Query syntax	212
Return format	212
Attribute summary	212

[SENSe:]DCONverter:ATTenuator	213
Command syntax	213
Example	213
Query syntax	213
Return format	213
Attribute summary	213
Additional information	213

[SENSe:]DCONverter:ATTenuator:AUTO	214
Command syntax	214
Example	214
Query syntax	214
Return format	214
Attribute summary	214
Additional information	214

[SENSe:]DCONverter:ATTenuator:AUTO: IMMEDIATE	215
Command syntax	215
Attribute summary	215
Additional information	215

[SENSe:]DCONverter:BAND	216
Command syntax	216

Example	216
Query syntax	216
Return format	216
Attribute summary	216
Additional information	216
[SENSe:]DCONverter:FREQuency	217
Command syntax	217
Example	217
Query syntax	217
Return format	217
Attribute summary	217
[SENSe:]DCONverter:IFFRequency?	218
Command Syntax	218
Query syntax	218
Return format	218
Attribute summary	218
Additional information	218
[SENSe:]DCONverter:IFGain	219
Command syntax	219
Example	219
Query syntax	219
Return format	219
Attribute summary	219
[SENSe:]DCONverter:IFGain:AUTO	220
Command syntax	220
Example	220
Query syntax	220
Return format	220
Attribute summary	220
Additional information	220
[SENSe:]DCONverter:IFGain:AUTO:	
IMMEDIATE	221
Command syntax	221
Attribute summary	221
Additional information	221
[SENSe:]DCONverter:L1BWidth	222
Command syntax	222
Example	222
Query syntax	222
Return format	222
Attribute summary	222

[SENSe:]DCONverter:L6BWidth	223
Command syntax	223
Example	223
Query syntax	223
Return format	223
Attribute summary	223
[SENSe:]DCONverter:LOPower	224
Command syntax	224
Example	224
Query syntax	224
Return format	224
Attribute summary	224
[SENSe:]DCONverter:LOSelect	225
Command syntax	225
Example	225
Query syntax	225
Return format	225
Attribute summary	225
[SENSe:]DCONverter:LOSelect:AUTO	226
Example	226
Query syntax	226
Return format	226
Attribute summary	226
[SENSe:]DCONverter:MEXT:BIAS	227
Command syntax	227
Example	227
Query syntax	227
Return format	227
Attribute summary	227
Additional information	227
[SENSe:]DCONverter:MEXT:BIAS:STATe	228
Command syntax	228
Example	228
Query syntax	228
Return format	228
Attribute summary	228
Additional information	228
[SENSe:]DCONverter:MMLO?	229
Command Syntax	229
Query syntax	229
Return format	229

Attribute summary	229
[SENSe:]DCONverter:PLO	230
Command syntax	230
Attribute summary	230
Additional information	230
[SENSe:]DCONverter:REFerence	231
Command syntax	231
Example	231
Query syntax	231
Return format	231
Attribute summary	231
Additional information	231
[SENSe:]DCONverter:TSENSitivity?	232
Command Syntax	232
Query syntax	232
Return format	232
Attribute summary	232
Additional information	232
[SENSe:]DCONverter:TUNE:PORT	234
Command syntax	234
Example	234
Query syntax	234
Return format	234
Attribute summary	234
[SENSe:]DETector:FREQuency	235
Command syntax	235
Example	235
Query syntax	235
Return format	235
Attribute summary	235
Additional information	235
[SENSe:]DETector:SELect	236
Command syntax	236
Example	236
Query syntax	236
Return format	236
Attribute summary	236
Additional information	236
[SENSe:]FFT:INPut:COUpling	238
Command syntax	238
Example	238

Query syntax	238
Return format	238
Attribute summary	238
[SENSe:]NOISe:BBGain	239
Command syntax	239
Example	239
Query syntax	239
Return format	239
Attribute summary	239
Additional information	239
[SENSe:]NOISe:FFT	240
Command syntax	240
Query syntax	240
Example	240
Return format	240
Attribute summary	240
Additional information	240
[SENSe:]NOISe:MEAStype	241
Command syntax	241
Example	241
Query syntax	241
Return format	241
Attribute summary	241
Additional information	241
[SENSe:]NOISe:PULSed	242
Command syntax	242
Example	242
Query syntax	242
Return format	242
Attribute summary	242
Additional information	242
[SENSe:]NOISe:QUADrature[:METHOD]	243
Command syntax	243
Example	243
Query syntax	243
Return format	243
Attribute summary	243
[SENSe:]RANGE:FFT:AVERage:MINimum	244
Command syntax	244
Example	244
Query syntax	244

Return format	244
Attribute summary	244
Additional information	244
[SENSe:]RANGE:FFT:SEGTable [:MEASurement][:QUALity]	245
Command syntax	245
Example	245
Query syntax	245
Return format	245
Attribute summary	245
Additional information	245
[SENSe:]RANGE:OFFSet	246
Example	246
Query syntax	246
Return format	246
Attribute summary	246
[SENSe:]RANGE:SWEPt:SEGTable [:MEASurement][:QUALity]	247
Command syntax	247
Example	247
Query syntax	247
Return format	247
Attribute summary	247
Additional information	247
[SENSe:]TSET:ATTenuator	248
Command syntax	248
Example	248
Query syntax	248
Return format	248
Attribute summary	248
Additional information	248
[SENSe:]TSET:ATTenuator:AUTO	249
Command syntax	249
Example	249
Query syntax	249
Return format	249
Attribute summary	249
Additional information	249
Command syntax	250
Example	250
Query syntax	250
Return format	250

Attribute summary	250
Additional information	250
Command syntax	251
Example	251
Query syntax	251
Return format	251
Attribute summary	251
Additional information	251
[SENSe:]TSET:LNAGain:METHod	252
Command syntax	252
Example	252
Query syntax	252
Return format	252
Attribute summary	252
Additional information	252
[SENSe:]TSET:LNAGain:MINimum	253
Command syntax	253
Example	253
Query syntax	253
Return format	253
Attribute summary	253
Additional information	253
[SENSe:]TSET:LPF	254
Command syntax	254
Query syntax	254
Example	254
Return format	254
Attribute summary	254
Additional information	254
[SENSe:]TSET:LPF:AUTO	255
Command syntax	255
Example	255
Query syntax	255
Return format	255
Attribute summary	255
Additional information	255
[SENSe:]TSET:PLL:ATTenuator	256
Command syntax	256
Query syntax	256
Example	256
Return format	256

Attribute summary	256
Additional information	256
[SENSe:]TSET:PLL:UNLock:IGNore	258
Command syntax	258
Query syntax	258
Example	258
Return format	258
Attribute summary	258
Additional information	258
Command syntax	259
Query syntax	259
Example	259
Return format	259
Attribute summary	259
Additional information	259

## 15 SOURce Commands

SOURce Commands Introduction	262
SOURce:CALibration:FM[:DEViation]	263
Command syntax	263
Example	263
Query syntax	263
Return format	263
Attribute summary	263
SOURce:CALibration:FM:INTernal:	
FREQuency	264
Command syntax	264
Example	264
Query syntax	264
Return format	264
Attribute summary	264
SOURce:CALibration:FREQuency[:CW FIXed]	265
Command syntax	265
Example	265
Query syntax	265
Return format	265
Attribute summary	265
SOURce:CALibration:POWer	
[:LEVel AMPLitude]	266
Command syntax	266
Example	266

Query syntax	266
Return format	266
Attribute summary	266
SOURce:CARRier:FREQuency[:CW FIXed]	267
Command syntax	267
Example	267
Query syntax	267
Return format	267
Attribute summary	267
SOURce:CARRier:POWer	
[:LEVel AMPLitude]	268
Command syntax	268
Example	268
Query syntax	268
Return format	268
Attribute summary	268
Additional information	268
SOURce:REFerence:FREQuency:DIVisor	269
Command syntax	269
Example	269
Query syntax	269
Return format	269
Attribute summary	269
Additional information	269
SOURce:REFerence:FREQuency:MULTiplier	270
Command syntax	270
Example	270
Query syntax	270
Return format	270
Attribute summary	270
Additional information	270
SOURce:REFerence:POWer	
[:LEVel AMPLitude]	271
Command syntax	271
Example	271
Query syntax	271
Return format	271
Attribute summary	271
Additional information	271
SOURce:RESidual:FREQuency[:CW FIXed]	272
Command syntax	272

Example	272
Query syntax	272
Return format	272
Attribute summary	272
SOURce:RESidual:FREQuency:CALCulate	273
Command syntax	273
Example	273
Query syntax	273
Return format	273
Attribute summary	273
Additional information	273
SOURce:RESidual:FREQuency:DETector:	
COUPled	274
Command syntax	274
Example	274
Query syntax	274
Return format	274
Attribute summary	274
Additional information	274
SOURce:REFerence:FREQuency:DIVisor	276
Command syntax	276
Example	276
Query syntax	276
Return format	276
Attribute summary	276
Additional information	276
SOURce:RESidual:FREQuency:MULTiplier	277
Command syntax	277
Example	277
Query syntax	277
Return format	277
Attribute summary	277
Additional information	277
SOURce:RESidual:POWER	
[:LEVel   AMPLitude]	278
Command syntax	278
Example	278
Query syntax	278
Return format	278
Attribute summary	278

## 16 STATus Commands

STATus Commands Introduction	280
Figure 17. Event status register 1	281
Figure 18. Event status register 2	282
STATus:ADVise:ENABLE	283
Command syntax	283
Example	283
Query syntax	283
Return format	283
Attribute summary	283
STATus:OPERation:CONDITION?	284
Command syntax	284
Query syntax	284
Return format	284
Attribute summary	284
Additional information	284
STATus:OPERation:ENABLE	285
Command syntax	285
Example	285
Query syntax	285
Return format	285
Attribute summary	285
Additional information	285
STATus:OPERation:EVENT?	286
Command syntax	286
Query syntax	286
Return format	286
Attribute summary	286
Additional information	286
STATus:OPERation:NTRansition	287
Command syntax	287
Example	287
Query syntax	287
Return format	287
Attribute summary	287
Additional information	287
STATus:OPERation:PTRansition	288
Command syntax	288
Example	288
Query syntax	288
Return format	288

Attribute summary	288
Additional information	288
STATUs:PRESet	289
Command syntax	289
Query syntax	289
Example	289
Attribute summary	289
Additional information	289
STATUs:QUEStionable:CONDition?	290
Command syntax	290
Query syntax	290
Return format	290
Attribute summary	290
Additional information	290
STATUs:QUEStionable:ENABLE	291
Command syntax	291
Example	291
Query syntax	291
Return format	291
Attribute summary	291
Additional information	291
STATUs:QUEStionable:[EVENT]?	292
Command syntax	292
Query syntax	292
Return format	292
Attribute summary	292
Additional information	292
STATUs:QUEStionable:NTRansition	293
Command syntax	293
Example	293
Query syntax	293
Return format	293
Attribute summary	293
Additional information	293
STATUs:QUEStionable:PTRansition	294
Command syntax	294
Example	294
Query syntax	294
Return format	294
Attribute summary	294
Additional information	294

## 17 SYSTem Commands

SYSTem Commands Introduction	296
SYSTem:ASSet:CALSource	297
Command syntax	297
Example	297
Query syntax	297
Return format	297
Attribute summary	297
Additional information	297
SYSTem:ASSet:CARRier	298
Command syntax	298
Example	298
Query syntax	298
Return format	298
Attribute summary	298
Additional information	298
SYSTem:ASSet:COUNter	299
Command syntax	299
Example	299
Query syntax	299
Return format	299
Attribute summary	299
Additional information	299
SYSTem:ASSet:DCONverter	300
Command syntax	300
Example	300
Query syntax	300
Return format	300
Attribute summary	300
Additional information	300
SYSTem:ASSet:DCONverter:USAGe	301
Command syntax	301
Example	301
Query syntax	301
Return format	301
Attribute summary	301
Additional information	301
SYSTem:ASSet:FFT	302
Command syntax	302
Example	302
Query syntax	302

Return format	302
Attribute summary	302
Additional information	302
SYSTem:ASSet:FFT:CUSTom[:SEGTable]	303
Command syntax	303
Example	303
Attribute summary	303
Additional information	303
SYSTem:ASSet:PSHifter	304
Command syntax	304
Query syntax	304
Example	304
Return format	304
Attribute summary	304
Additional information	304
SYSTem:ASSet:REFerence	305
Command syntax	305
Example	305
Query syntax	305
Return format	305
Attribute summary	305
Additional information	305
SYSTem:ASSet:RESidual	306
Command syntax	306
Query syntax	306
Example	306
Return format	306
Attribute summary	306
Additional information	306
SYSTem:ASSet:SLAVe:SOURce	307
Command syntax	307
Example	307
Query syntax	307
Return format	307
Attribute summary	307
Additional information	307
SYSTem:ASSet:SLAVe:SOURce:PORT	308
Command syntax	308
Example	308
Query syntax	308
Return format	308

Attribute summary	308
Additional information	308
SYSTem:ASSet:SWANalyzer	309
Command syntax	309
Example	309
Query syntax	309
Return format	309
Attribute summary	309
Additional information	309
SYSTem:ASSet:SWANalyzer:CUSTom [:SEGTable]	310
Command syntax	310
Example	310
Attribute summary	310
Additional information	310
SYSTem:ASSet:TBASe	311
Command syntax	311
Example	311
Query syntax	311
Return format	311
Attribute summary	311
Additional information	311
SYSTem:ASSet:TSET	312
Command syntax	312
Example	312
Query syntax	312
Return format	312
Attribute summary	312
Additional information	312
SYSTem:ERRor?	313
Command syntax	313
Query syntax	313
Example	313
Attribute summary	313
Additional information	313
Table 3. SCPI Error Messages	314
SYSTem:GUI:LLOCKout[:STATe]	316
Command syntax	316
Example	316
Attribute summary	316
Additional information	316

SYSTem:GUI:REMote[:STATe]	317
Command syntax	317
Example	317
Query syntax	317
Return format	317
Attribute summary	317
Additional information	317
SYSTem:HELP:HEADers?	318
Command syntax	318
Query syntax	318
Return format	318
Attribute summary	318
Additional information	318
SYSTem:PATH:CARRier	319
Command syntax	319
Example	319
Query syntax	319
Return format	319
Attribute summary	319
SYSTem:PATH:DCBBanalyzer	320
Command syntax	320
Example	320
Query syntax	320
Return format	320
Attribute summary	320
Additional information	320
SYSTem:PATH:FFTAnalyzer	321
Command syntax	321
Example	321
Query syntax	321
Return format	321
Attribute summary	321
Additional information	321
SYSTem:PATH:SWANalyzer	322
Command syntax	322
Example	322
Query syntax	322
Return format	322
Attribute summary	322
Additional information	322
SYSTem:PATH:TVCO	323

Command syntax	<a href="#">323</a>
Example	<a href="#">323</a>
Query syntax	<a href="#">323</a>
Return format	<a href="#">323</a>
Attribute summary	<a href="#">323</a>
SYSTem:TStArt?	<a href="#">324</a>
Command syntax	<a href="#">324</a>
Query syntax	<a href="#">324</a>
Return format	<a href="#">324</a>
Attribute summary	<a href="#">324</a>
SYSTem:VERSion?	<a href="#">325</a>
Command syntax	<a href="#">325</a>
Query syntax	<a href="#">325</a>
Return format	<a href="#">325</a>
Attribute summary	<a href="#">325</a>
Additional information	<a href="#">325</a>

# 1 **SCPI Interface**

- Introduction [38](#)
- Configuring the SCPI Interface [39](#)
- Starting the SCPI Interface [44](#)
- Starting the SCPI Interface Programmatically [47](#)



## Introduction

Standard Commands for Programmable Instruments (SCPI) defines how you communicate with an instrument from a computer. It is a programming language designed specifically for electronic test and measurement instruments. SCPI standards are built on the IEEE-488.2 Standard Codes and Formats. For more information on SCPI, visit <http://www.scpiconsortium.org>.

The SCPI programming commands presented in this manual are used with the E5500 Phase Noise Measurement System software, which operates in all of the E5500 series of phase noise measurement systems (including the E5505A). The E5500 programming commands comply with the SCPI standards.

## Configuring the SCPI Interface

The SCPI interface provides connectivity between the E5500 phase noise measurement (software) subsystem and your application programming environment. Multiple types of interfaces and protocols are supported. Before using an interface with the E5500 Phase Noise System Measurement software, some system configuration may be required. You need to configure only the interfaces you plan to use.

Once connected and configured, use the SCPI interface to open other interfaces and send SCPI commands to the phase noise subsystem.

## Configuring Telnet and sockets interfaces

These interfaces use TCP/IP protocol through a LAN connection. In order to use these interfaces, you must have Windows® networking installed and configured. If you want to control the E5500 phase noise measurement subsystem from a remote computer, an appropriate LAN card must also be installed and configured.

## Configuring the RS-232 interface

This interface provides direct serial port connection using a null-modem cable. COM port settings as set by the Windows operating system configuration utility are used. To view or modify settings click:

**Start > Settings > Control Panel > Ports.**

## Configuring the VXI-11 interface


This interface uses VXI-11 protocol which provides full GPIB emulation through a LAN connection. It requires a software simulated GPIB card called an internal instrument installed and configured in Agilent I/O Libraries. The SCPI interface is then used to open this simulated GPIB card and connect it to the Phase Noise Subsystem. The Agilent I/O Libraries software which adds the internal instrument interface is included on the E5500 CD-ROM.

### NOTE

The Agilent I/O libraries version M and the I/O upgrade must be installed before beginning this procedure. Refer to the *E5505A Phase Noise Measurement System Installation Guide* for more information.

## 1 SCPI Interface

**Figure 1** shows the relationship between the E5500 phase noise measurement subsystem, the SCPI Interface, the I/O Libraries Internal Instrument, and the user's application program running on either the same or a remote computer.

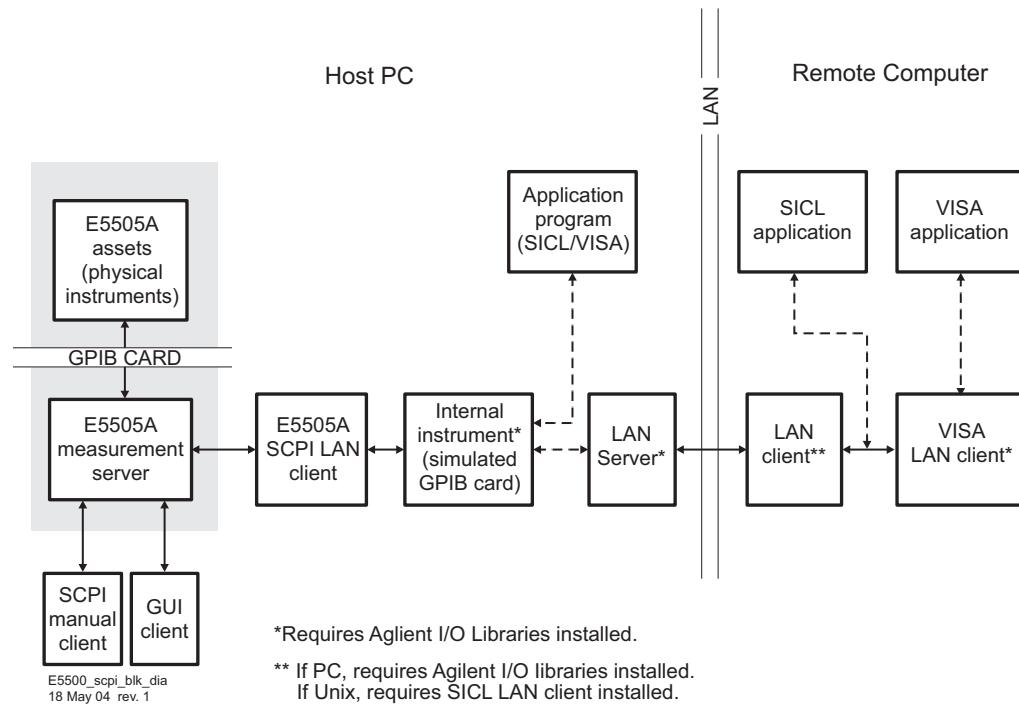

**Figure 1** E5500 block diagram


Use the Agilent I/O Libraries I/O Config utility to configure an Internal Instrument interface before attempting to open a VXI-11 interface with the SCPI remote interface.

- 1 Use the Windows start menu as in [Figure 2](#) to navigate to I\_O Config.



**Figure 2** E5500 navigate to I\_O Config


- 2 In the Interface Configuration Application window, select **Internal Instrument** in the left pane and click the **Configure** button ([Figure 3](#)).

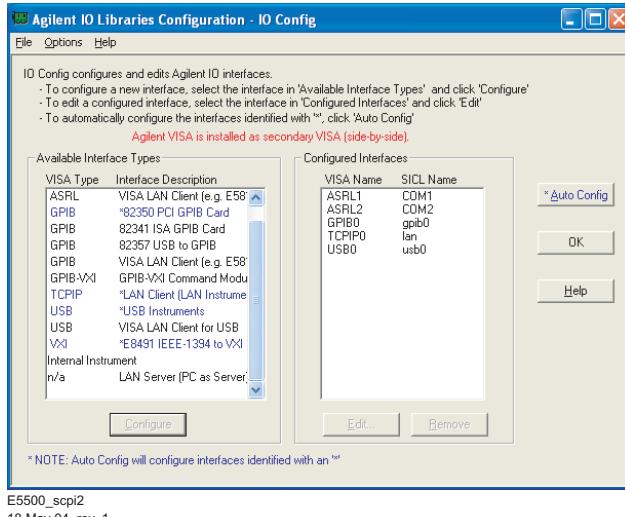

**Figure 3** Select internal instrument

## 1 SCPI Interface


- 3 Click OK to accept the default settings ([Figure 4](#)). The software will choose the next available “gpib(x)” number (usually gpib7 and gpib1).

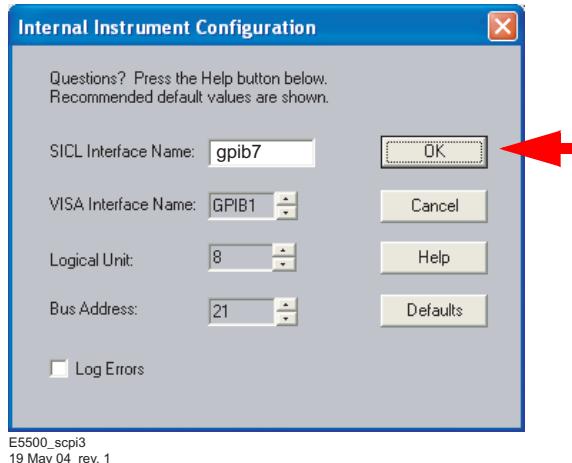

**Figure 4** Accept default settings

### NOTE

The internal instrument required to use the SCPI (LAN) Client is added to the list in the right pane (Configured Interfaces). See [Figure 5](#) on page 42.

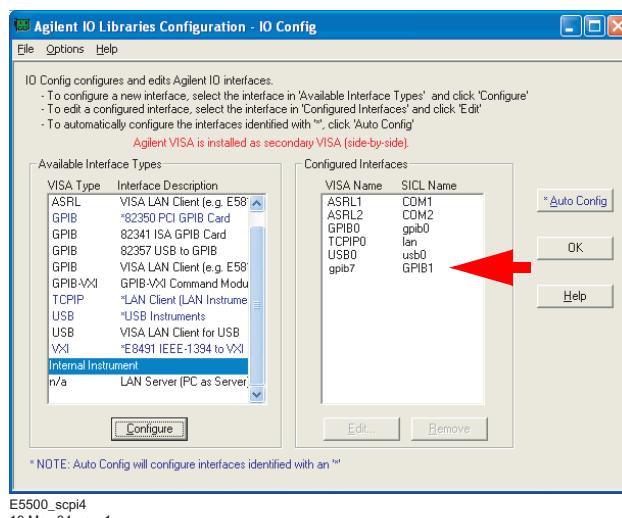


**Figure 5** Configured default settings

## Activating the LAN server (optional)

Activating the LAN Server is only required if you wish to control the E5500 phase noise measurement system using the SCPI VXI-11 interface from a remote computer.

Use the Windows start menu as in [Figure 6](#) to navigate to the LAN Server.

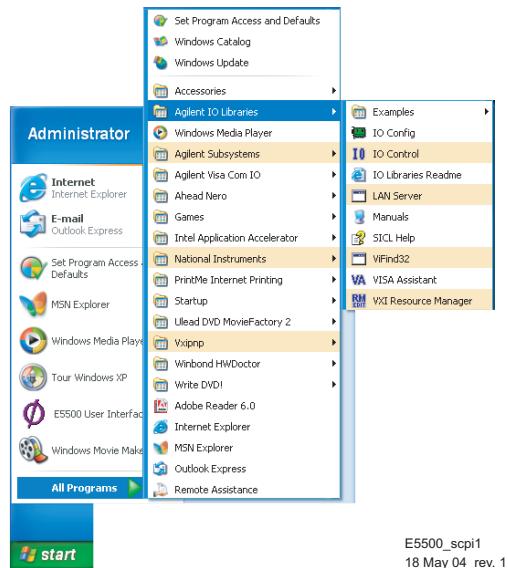


**Figure 6** Navigate to LAN server

- 4 The LAN Server dialog box appears. This dialog box does not display any information, but it needs to be active for the LAN Server to function. The window can be minimized (button in the upper-right corner of the dialog box). The LAN Server is now ready to communicate with a remote PC or UX workstation.

## Starting the SCPI Interface

- 1 Use the Windows start menu as in [Figure 7](#) to navigate to SCPI Interface.

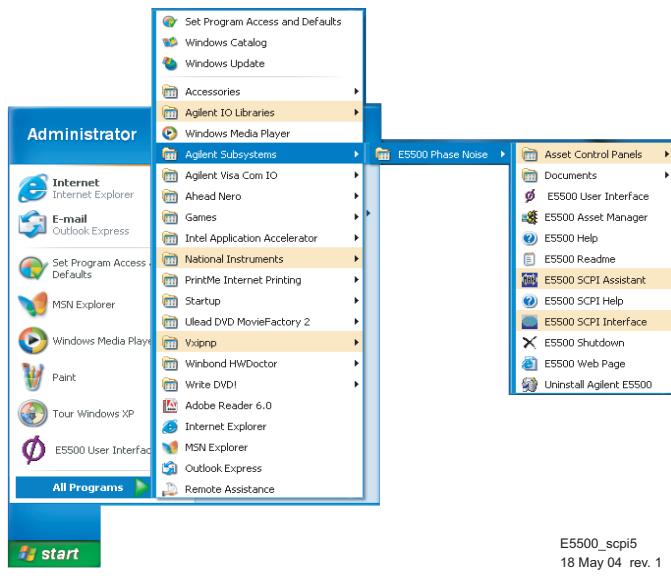

**Figure 7** Navigate to SCPI interface


- 2 The **SCPI Interface Selections** dialog box appears.

### NOTE


This dialog box is used to open one or more interfaces to the SCPI Interface. These interfaces provide connectivity between the Phase Noise Subsystem and the user's application programming environment. Once connected, SCPI commands may be sent to the Subsystem through the SCPI Interface as if it is an instrument on a GPIB bus.

- Telnet - TCP/IP protocol, requires installed and configured networking software.
  - Sockets - TCP/IP protocol, requires installed and configured networking software.
  - RS-232 - Serial COM Port Interface (direct connection)
  - VXI-11 - VXI-11 protocol, requires Agilent I/O Libraries software with a "Internal Instrument" type interface configured. For more information, see "[Configuring the VXI-11 interface](#)" on page 39.
- 3 Choose which protocol you wish to use by checking either **Telnet Enable**, **Sockets Enable**, **RS-232 Enable** or **VXI-11 Enable** ([Figure 8](#) on page 45).
  - 4 If you selected **VXI-11 Enable**, in the **Select SICL Interface** pull-down list, select **gpib (x)** (**gpib7**, for example). Only the Internal Instrument type interfaces defined in "[Introduction](#)" on page 38, will be listed. You may also change the bus address of the subsystem if desired (default is 0).

**5** Click the **OK** button.

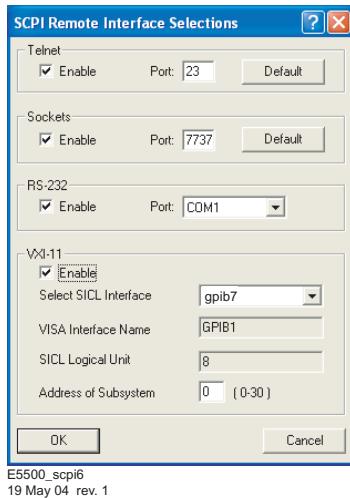

**Figure 8** Choosing the interface

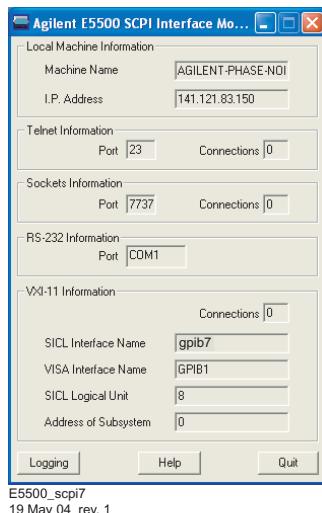

**Figure 9** SCPI interface information


The selected interface is now open and connected to the E5505A phase noise measurement server. Local machine (PC) information appears in the top section, the bottom sections contain information about the selected interface(s).

#### NOTE

You must open an interface with the SCPI Interface **before** running any application software.

## SCPI logging function

- 1 Click the **Logging** button shown in Figure 9. The SCPI Logging dialog box appears as shown in Figure 10.

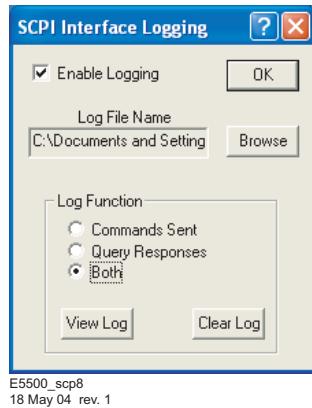

**Figure 10** E5500 LAN client logging

- 2 Click the **OK** button.

When enabled, the SCPI Interface Logging dialog box allows you to log Commands Sent, or Query Responses, or Both. The logged functions can be saved as a text file (\*.txt) using a name and directory of your choice.

## Starting the SCPI Interface Programmatically

The SCPI Interface can be started programmatically from a DOS command prompt, a WinNT shortcut, or from a program using the following syntax:

```
lanSCPIclient.exe \driver ("name" | telnet | sockets | serial)
```

Only one type of interface may be opened with the command line. The \driver option takes *one* of the following arguments:

**"name"** Opens a VXI-11 interface where **"name"** is a quoted string SICL interface name to open.

Example: lanScpiClient.exe \driver "gpib7"

**telnet** Opens a telnet interface. The port setting last opened is used.

Example: lanScpiClient.exe \driver telnet

**sockets** Opens a sockets interface. The port setting last opened is used.

Example: lanScpiClient.exe \driver sockets

**serial** Opens a RS-232 interface. The port setting last opened is used.

Example: lanScpiClient.exe \driver serial

## DOS command prompt example

### Telnet

```
"C:\Program Files\Agilent\Measurement and Stimulus Subsystems\
E5500 Phase Noise\lanSCPIclient.exe"\driver telnet
```

### Sockets

```
"C:\Program Files\Agilent\Measurement and Stimulus Subsystems\
E5500 Phase Noise\lanSCPIclient.exe"\driver sockets
```

### Serial (RS-232)

```
"C:\Program Files\Agilent\Measurement and Stimulus Subsystems\
E5500 Phase Noise\lanSCPIclient.exe"\driver serial
```

### VXI-11

```
"C:\Program Files\Agilent\Measurement and Stimulus Subsystems\
E5500 Phase Noise\lanSCPIclient.exe"\driver "gpib7"
```

## 1 SCPI Interface

## 2 **SCPI Assistant**

Starting the SCPI Assistant 50




**Agilent Technologies**

## Starting the SCPI Assistant

The Agilent Technologies SCPI assistant is useful for program development, allowing the user to enter one SCPI command at a time and view queries.

Use the Windows start menu as in [Figure 11](#) to navigate to SCPI assistant.

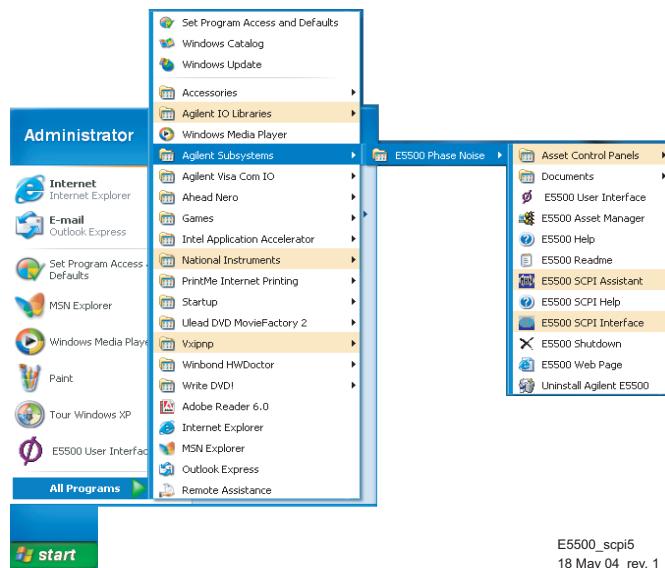


**Figure 11** Navigate to SCPI assistant

The SCPI Assistant Interface ([Figure 12](#)) allows the user to enter SCPI commands directly using the keyboard and then send the commands directly using the keyboard's Enter key.

A **Quick Reference Guide (QRG)** window lists the SCPI command which (by double-clicking) can be placed in the SCPI command window and sent by using the keyboard's Enter key. To view the QRG (Quick Reference Guide), click the **View QRG** button. The QRG can be printed using the standard Window printing capability.


Query responses appear in the Query Response Window.

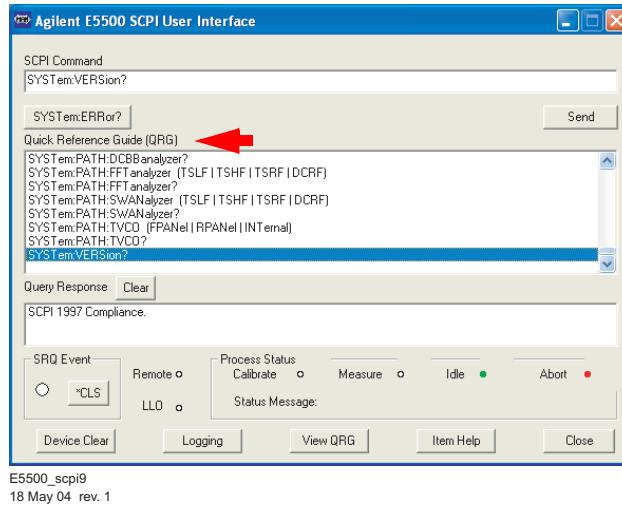

**Figure 12** SCPI assistant interface

## SCPI logging function

Click the **Logging** button (Figure 12). The **LAN Client Logging** dialog box appears (Figure 13). When enabled, this dialog box allows you to log Commands Sent, or Query Responses, or Both. The logged functions can be saved as a text file (\*.txt) using a name and directory of your choice.

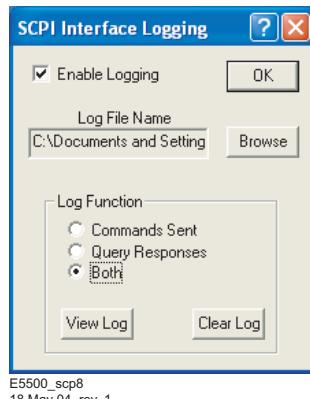

**Figure 13** E5500 LAN client logging

- Click the **OK** button.



## 3

# SCPI Program Examples

[Application Environment Setup](#) [54](#)

[SCPI Programming](#) [56](#)

[HTBasic for Windows Program Example](#) [58](#)



## Application Environment Setup

Application software communicates with the E5505A system measurement server thorough the interface opened with the SCPI Interface. The SCPI Interface must open the selected interface before running your application software. Information about the selected interface and the host PC is displayed in the SCPI Interface Monitor dialog. The information your application needs to connect to this interface depends upon the type of I/O your application supports (SICL or VISA), and if your application is running on the same PC as the E5505A system or a remote computer.

The following are language specific examples of application setup. In all cases the SCPI interface has opened a VXI-11 interface with the SICL Interface Name of "gpib8" and the address of subsystem "0".

### HTBasic for Windows on same PC or remote PC

The autostart (autost) file must use the HPIBS driver to open the interface as follows:

**Same PC as E5505A:** LOAD BIN "HPIBS; DEV gpib8 ISC 7"!

**Remote PC name or IP:** LOAD BIN "HPIBS; DEV lan[pc52]:gpib8 ISC 7"!

- "pc52" is the name of the PC running the E5505A. You may also use an IP address here. "gpib8" is the SICL interface name opened with the SCPI LAN Client.

**NOTE**

Using a remote PC requires installing Agilent I/O Libraries LAN CLIENT on the remote PC.

---

Your program would then look like:

```
OUTPUT 700; "*IDN?"  
ENTER 700; Id$
```

### RMBUX on remote workstation

Users **RMBUX ~/.rmrc** file must open interface as follows:

```
INTERFACE 9="lan[pc52]:gpib8"; normal
```

- "pc52" is the name of the pc running the E5505A system. You may also use an IP address here. "gpib8" is the SICL interface name opened with the SCPI LAN Client.

**NOTE**

RMBUX Requires that the SICL LAN CLIENT be installed on your UNIX system, see your UNIX system administrator.

Your program would then look like:

```
OUTPUT 900; "*IDN?"  
ENTER 900; ID$
```

## Agilent Vee on same PC or remote PC

Use the Instrument Manager in the I/O menu to configure an interface and device as defined in the SCPI LAN Client. If on a remote computer, add the name or IP address of the PC running the E5505A system in the Gateway: pane.



**Figure 14** Add IP address

## SCPI Programming

Generally, any E5500 program must perform these tasks:

- Set up the measurement definition
- Set up the device under test (DUT)<sup>1</sup>
- Initiate measurement and determine when complete
- Read the data from the measurement
- Process, display and store the data<sup>\*</sup>

As with most programming tasks there is more than one method to accomplish these tasks. Several methods are discussed in this document.

### Set up the measurement definition

Before programming a measurement you should first make the desired measurement manually using the Measurement Client GUI. Once you have the measurement defined and are satisfied with the results, save the measurement setup using the File > Save As menu selection. This saves the complete measurement definition and the data from the last measurement performed to a file. A file should be saved for each Measurement Type (Absolute, Noise, etc.) you wish to make. A few parameters (for example, carrier frequency) may be adjusted after recalling a measurement setup file.

Your program can then load the desired measurement file using the command MMEMORY:LOAD[:ALL] (“path\name.pnm”), adjust any parameters as necessary and begin the measurement. This is the simplest method of measurement setup under program control.

**NOTE**

Do not use special characters, including the underscore ( \_) character, in path names.

---

Users who do not wish to use pre-defined measurement files to setup their measurement should still use the Measurement Client GUI to develop and successfully make their measurement. Start from the File > New menu state and then adjust all required parameters. The command \*RST is the equivalent of File > New and should begin the setup section of your program followed by the commands for all adjusted parameters.

<sup>\*</sup> These tasks are user specific and are not discussed in this document.

## Initiate measurement and determine when complete

The SCPI command INITiate[:IMMediate][:ALL] begins a calibration and measurement sequence. A wait of approximately 15 seconds is recommended after issuing this command, as the E5505A system requires nearly 100% of the CPU time when initializing the system assets (instruments).

Once a measurement is begun, the SCPI status system may be used to monitor measurement progress and determine when complete. This may be done by polling the Operation Condition register with the query, STATus:OPERation:CONDition? and waiting for the “Idle” bit. Another method is to send \*OPC after the INITiate command which will set the “Operation Complete” bit of the Event Status Register (\*ESR?).

System errors should be checked while measuring or at least when a measurement is complete using the SCPI query SYSTem:ERRor?. The error queue should be read until message 0, “No error” is received and appropriate action, if any taken upon non 0 errors. In addition to standard SCPI errors, the following E5500 error messages may occur:

- *100-199 Abort messages* - measurement aborted.
- *200-299 Pause point messages* - measurement paused. This may also trigger an abort if PAUSE:ABORT:AUTO is ON(default=ON).
- *300-499 Status messages* - informative only, no action required. Only reported if STATus:ADVise:ENABLE is ON (default=OFF).
- *500-599 Warning messages* - advisory but measurement can proceed on its own.

## Read the data from the measurement

After completing a measurement and checking system errors you are ready to read the data. The simplest method of data output uses the SCPI queries [:SENSe]:DATA:HEADER:POINTs? and [:SENSe]:DATA?. The POINTs? query returns the total number of points measured. The DATA? query returns one line per point in the format: frequency, amplitude, spur flag. The amplitude is always in the Spectral density of phase fluctuations (dB/Hz) format and the spur flag (0/1) is 1 if the data point is a spur.

Commands in the CALCulate: SCPI tree can be used to output subsets of the data, data in other formats, or processed data.

## HTBasic for Windows Program Example

The following program example demonstrates use of the above techniques in a HTBASIC program. It runs with your system in Demo Mode. The program recalls a measurement setup file and then makes measurements at several carrier frequencies. For information about HTBASIC for Windows, refer to the URL, <http://www.htbasic.com>.

Lines to note:

- 210 Timeout - a minimum 5 second timeout period is recommended.
- 570 Recall measurement setup file.
- 650 Set carrier frequency.
- 710 Begin measurement sequence.
- 900 Wait for measurement to complete subroutine. This polls the Status Operation Condition register to monitor measurement progress.
- 1050 Check System Errors subroutine.
- 1280 Read data subroutine. This uses SENSe:DATA? output.

```
-----  
10 !      RE-SAVE "DEMO"  
20 ! ****  
30 ! * E5500 Phase Noise Measurement Subsystem  
40 ! *  
50 ! * Demonstration program to setup and initiate a  
60 ! * measurement and then output the data.  
70 ! *  
80 ! *      Copyright 2004 Agilent Technologies  
90 ! *  
100 ! ****  
110 !  
120 OPTION BASE 1  
130 INTEGER Isc,Soc,Err,I,J,M,Abort_flg,Points  
140 DIM Msg$[160],Path$[80],File$(5)[30],Freq$(5)[15]  
150 !  
160 Isc=8           ! Interface select code as set in the autost file.  
170 ASSIGN @Pn TO 800 ! Address of E5500. Always 00.  
180 !  
190 ! Initialize system.  
200 !  
210 ON TIMEOUT Isc,5 GOTO Time_out ! Recommend 5 second timeout.  
220 CLEAR SCREEN  
230 OUTPUT @Pn;"*RST; *CLS; STAT:PRES; *IDN?"  
240 ENTER @Pn;Msg$  
250 PRINT Msg$  
260 ! OUTPUT @Pn;"STAT:ADVise:ENABLE ON" ! Optional enable status  
messages.  
270 ! -----  
280 ! Load measurement setup file and frequency arrays.  
290 ! -----  
300 !  
310 ! Measurement setup file path and names.
```

```

320 Path$="c:\Program Files\Agilent\Measurement and Stimulus\E5500\
330 DATA Demomode.pnm, Confidence.pnm, EOD
340 !
350 I=1
360 READ File$(I)
370 WHILE File$(I)<>"EOD"
380 I=I+1
390 READ File$(I)
400 END WHILE
410 !
420 ! Carrier frequencies to measure for each setup.
430 DATA 500E6, 900E6, EOD
440 !
450 I=1
460 READ Freq$(I)
470 WHILE Freq$(I)<>"EOD"
480 I=I+1
490 READ Freq$(I)
500 END WHILE
510 ! -----
520 ! Start of measurement loop.
530 ! -----
540 I=1
550 WHILE File$(I)<>"EOD"      ! Load a measurement setup file.
560 !
570 OUTPUT @Pn;"MMEM:LOAD ""&Path$&File$(I) &"""
580 PRINT
590 PRINT "Measurement setup: ";File$(I)
600 GOSUB Read_err ! Check for file load errors.
610 WAIT 1
620 J=1
630 WHILE Freq$(J)<>"EOD"      ! Set carrier frequency and measure.
640 !
650 OUTPUT @Pn;"SOUR:CARR:FREQ "&Freq$(J)
660 !
670 ! Code to setup Device Under Test goes here.
680 !
690 Restart: Abort_flg=0
700 !
710 OUTPUT @Pn;"INIT:ALL"      ! Start new calibration & measurement.
720 !
730 PRINT "      Measuring carrier at: ";Freq$(J); " Hz"
740 GOSUB Wait_until_done ! Monitor status and errors.
750 !
760 ! Read the data if measurement was sucessful.
770 IF NOT Abort_flg THEN GOSUB Read_data
780 !
790 J=J+1
800 END WHILE
810 I=I+1
820 END WHILE
830 !
840 !
850 LOCAL @Pn
860 DISP "End of Program."
870 STOP ! End of main program.
880 ! -----

```

### 3 SCPI Program Examples

```
890 !
900 Wait_until_done:      !
910 REPEAT
920 DISP ""
930 WAIT 1
940 OUTPUT @Pn;"STAT:OPER:COND?"
950 ENTER @Pn,Soc
960 IF BIT(Soc,0) THEN DISP "Calibrating"
970 IF BIT(Soc,4) THEN DISP "Measuring"
980 IF BIT(Soc,8) THEN DISP "Paused"
990 IF BIT(Soc,9) THEN DISP "Idle"
1000 GOSUB Read_err
1010 WAIT 1
1020 UNTIL BIT(Soc,9) ! Idle state
1030 RETURN
1040 !
1050 Read_err:!
1060 REPEAT
1070 OUTPUT @Pn;"SYST:ERR?"
1080 ENTER @Pn,Err,Msg$
1090 IF Err<>0 THEN
1100 BEEP 300,.1
1110 PRINT " ";Err;Msg$
1120 IF Err=-250 THEN ! File error
1130 PRINT
1140 PRINT "File load error! Check path, file name and file exists."
1150 PRINT Path$&File$(I)
1160 LOCAL @Pn
1170 STOP
1180 END IF
1190 IF Err>=100 AND Err<=199 THEN ! Abort messages.
1200 Abort_flg=1
1210 INPUT "Measurement Aborted! Try again? (Y/N)",Ans$
1220 IF UPC$(Ans$[1,1])="Y" THEN GOTO Restart
1230 END IF
1240 END IF
1250 UNTIL Err=0 ! No error
1260 RETURN
1270 !
1280 Read_data: !
1290 OUTPUT @Pn;"DATA:HEAD:POIN?"
1300 ENTER @Pn,Points
1310 DISP "Reading";Points;" Data Points..."
1320 ALLOCATE Trace_data(Points,3)
1330 OUTPUT @Pn;"SENS:DATA?" ! Data triples - freq, amplitude, spur flag
1340 ENTER @Pn;Trace_data(*)
1350 !
1360 ! Data processing, storage or display code goes here.
1370 !
1380 PRINT " Point 1 =";Trace_data(1,2);"db @";Trace_data(1,1);"Hz"
1390 PRINT " Point";Points;"=";Trace_data(Points,2);"db
@";Trace_data(Points,1);"Hz"
1400 !
1410 DEALLOCATE Trace_data(*)
1420 DISP ""
1430 RETURN
1440 !
```

```
1450 Time_out: !
1460 BEEP 300,.2
1470 PRINT
1480 PRINT "*** Timeout Error! *** Check system and try again."
1490 !
1500 END
```

### **3 SCPI Program Examples**

4

## E5500 SCPI Commands

Syntax Conventions 64

Status Registers 65

Full Command List 68



## Syntax Conventions

**Table 1** Notation conventions and definitions

Convention	Additional information
< >	Angle brackets indicate values entered by the programmer
	"Or" indicates a choice of one element from a list. For example, but not both
[ ]	Square brackets indicate that the enclosed items are optional.
{ }	When several items are enclosed by braces, one, and only one of these elements must be selected.
~	A tilde Indicates a valid range of values
Integer	An ASCII string representing an integer. This is defined by the IEEE 488.2 <NR1> format.
Real	An ASCII string representing a real number. This is defined by the IEEE 488.2 <NR2> or <NRF> formats.
NA	not Applicable.

- If "Command Only" is not listed, the command can be issued as a query by including the question mark "?" character. For example,

:CALibrate:DETector:CONSTant

- The command can be sent as a query by sending:

:CALibrate:DETector:CONSTant?

- A colon (:) indicates branching points on the command tree
- A semicolon (;) sends multiple commands within a single program message. The command parser assumes the second command comes from the same branch as the preceding command. Use ; to reset the command parser to the base of the command tree.

## Status Registers

### Event Status Register (\*ESR?) Mask is \*ESE (value)

```

bit 0 = 1 = Operation Complete
bit 1 = 2 = Request Control
bit 2 = 4 = Query Error
bit 3 = 8 = Device Dependent Error. (Summary of QSR bits 9,10,11)
bit 4 = 16 = Execution Error. All API call error returns.
bit 5 = 32 = Command Error
bit 6 = 64 = User Request
bit 7 = 128 = Power On

```

### Status Byte (\*STB?) Mask is \*SRE (value)

```

bit 0 = 1 = Not Used
bit 1 = 2 = Not Used
bit 2 = 4 = Error/Event Queue
bit 3 = 8 = Summary of Questionable Status Register
bit 4 = 16 = MAV (Message Available)
bit 5 = 32 = Summary of Standard Event Status Register
bit 6 = 64 = RQS (SRQ State)
bit 7 = 128 = Summary of Operation Status Register

```

### Status Operation Register (STATus:OPERation:CONDition?)

```

bit 0 = 1 = Calibrating
bit 1-3 = Not Used
bit 4 = 16 = Measuring
bit 5-7 = Not Used
bit 8 = 256 = Paused
bit 9 = 512 = Idle
bit 10-15 = Not Used

```

### Status Questionable Register (STATus:QUESTIONable:CONDition?)

```

bit 0-8 = Not Used
bit 9 = 512 = Warning message available.
bit 10 = 1024 = Pause message available
bit 11 = 2048 = Abort message available
bit 12 = 4096 = Server Status message available.
bit 13-15 = Not Used

```


### Overlapped commands which start Pending Operations.

These are the only commands to which \*OPC, \*OPC? and \*WAI apply:


```

INITiate:CALibrate      (Calibrate)
INITiate:MEASure        (Measure)
INITiate:IMMediate:ALL  (Calibrate and Measure)

```

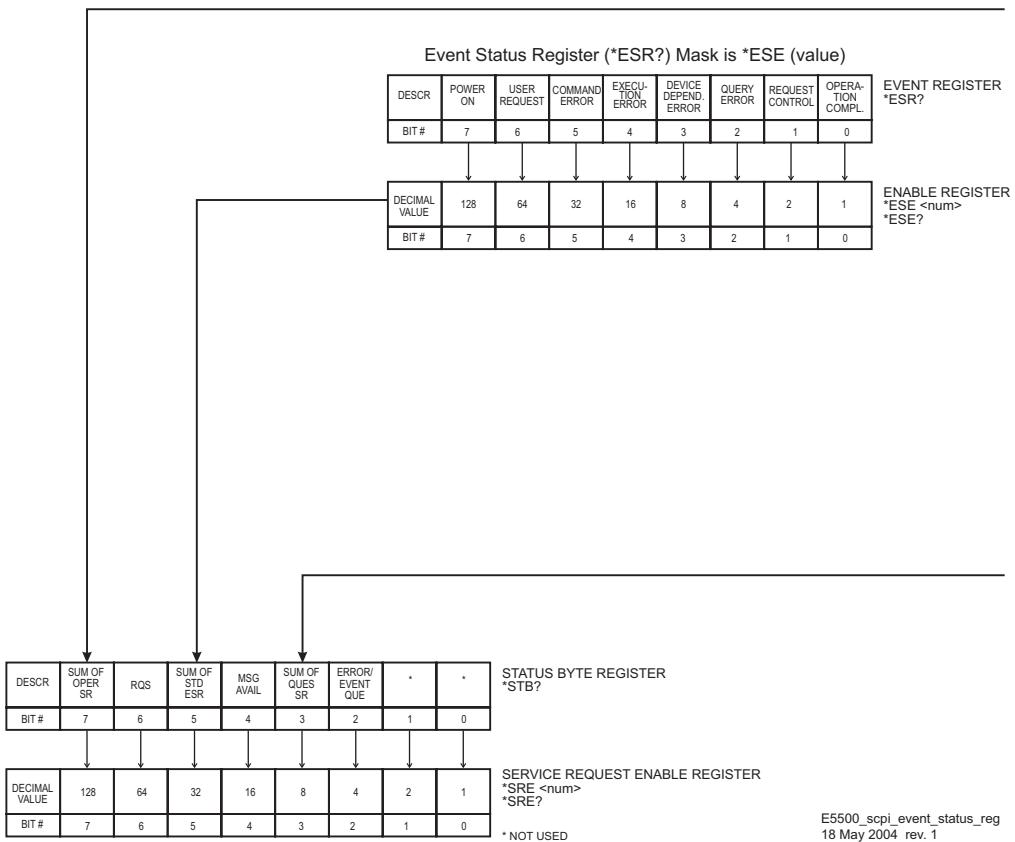

**Figure 15** Event status register 1

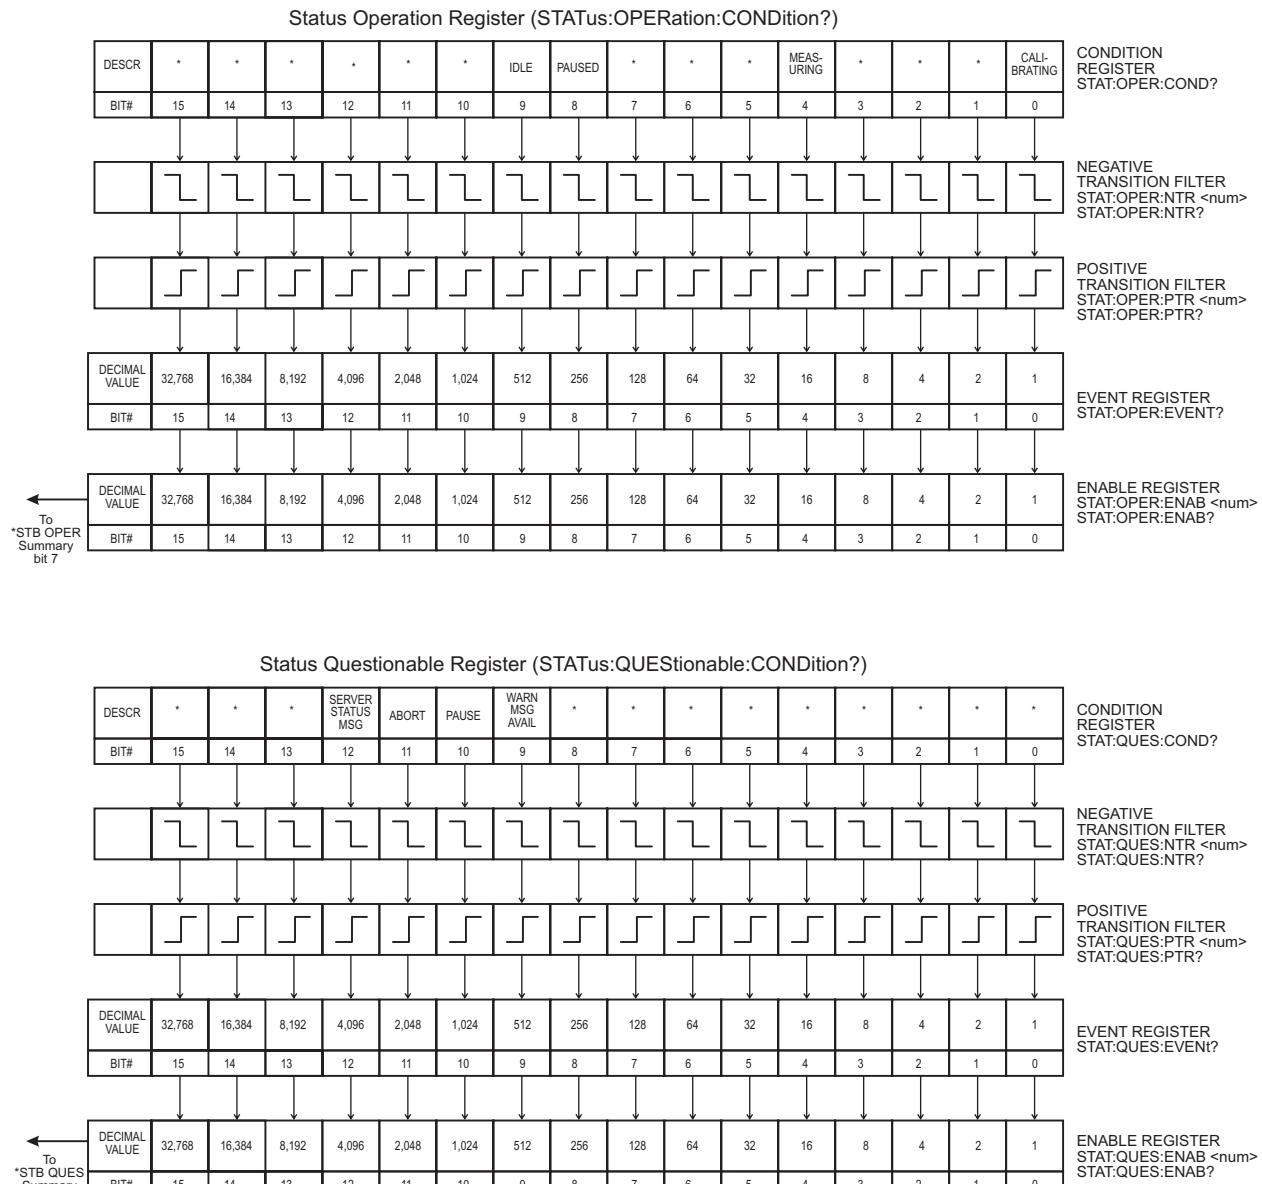**Figure 16** Event status register 2

## Full Command List

### NOTE

- Characters in lower case may be omitted.
- Commands within square brackets [.] are optional.
- Parentheses mark places where data parameters are required. Choose one from the list provided or enter a numeric value.
- Allowed Terminators: DB, mA, Hz, KHz, MHz, GHz.
- Default Terminators: If none of the above are provided, the entry will be assumed to be in fundamental units of measure, which includes: dB, Hz, etc.
- Numeric values: Exponential notation is accepted along with simple integers. i.e. 234, -139.34E+6

### Format of measurement data output

Measured Data

SENSe:DATA:HEADER:POINTs?	Returns Number of points.
SENSe:DATA?	

Returns triples with each element separated by a comma and terminated by cr/lf.

Each triple consists of the "frequency, amplitude and spur flag".

Processes Data

CALCulate:DATA:HEADER:POINTs?	Returns the number of points.
CALCulate:DATA?	Return varies with CALCulate:VIEW: setting.
CALCulate:VIE:SPURtable	Returns "frequency, amplitude" per point.
CALCulate:VIEW:TRACe	Returns "amplitude" per point.
CALCulate:VIEW:XYData	Returns "frequency, amplitude, spur_flag" per point.

### SCPI commands

```
*CLS
*ESE  (value)
*ESE?
*ESR?
*IDN?
*OPC
*OPC?
*RST
*SRE  (value)
*SRE?
*STB?
*TST?
*WAI
```

**ABORt**

ABORT

**CALCulate**

```

CALCulate:ACCumulated[:PHASE]? (tau, start-offset, stop-offset)
CALCulate:AVARiance? (tau, Frequency offset)
CALCulate:CFSCale (value)
CALCulate:CFSCale?
CALCulate:DATA?
CALCulate:DATA:HEADer:POINTs?
CALCulate:DIPower (value)
CALCulate:DIPower?
CALCulate:F2OScillator[:COMPARE] ("inFileA", "inFileAB",
"outFile", "title")
CALCulate:F3OScillator[:COMPARE] ("inFileAB", "inFileAC", "inFileBC",
"outFileA", "outFileB", "outFileC", "titleA", "titleB", "titleC")
CALCulate:INTegral? (start-offset, stop-offset)
CALCulate:INTegral:TYPE (NORMAL | CCITT)
CALCulate:INTegral:TYPE?
CALCulate:LIMit:NOISE:MAXimum (segment#, start_freq, start_amplitude,
stop_freq, stop_amplitude)
CALCulate:LIMit:NOISE:MAXimum? (segment_number)
CALCulate:LIMit:NOISE:MAXimum:DELETE (segment_number)
CALCulate:LIMit:NOISE:MAXimum:DELETE:ALL
CALCulate:LIMit:NOISE:MAXimum:DISPLAY (0 | OFF | 1 | ON)
CALCulate:LIMit:NOISE:MAXimum:DISPLAY?
CALCulate:LIMit:NOISE:MAXimum:FAIL? (segment_number)
CALCulate:LIMit:NOISE:MAXimum:FAIL:ALL?
CALCulate:LIMit:NOISE:MINimum (segment#, start_freq, start_amplitude,
stop_freq, stop_amplitude)
CALCulate:LIMit:NOISE:MINimum? (segment_number)
CALCulate:LIMit:NOISE:MINimum:DELETE (segment_number)
CALCulate:LIMit:NOISE:MINimum:DELETE:ALL
CALCulate:LIMit:NOISE:MINimum:DISPLAY (0 | OFF | 1 | ON)
CALCulate:LIMit:NOISE:MINimum:DISPLAY?
CALCulate:LIMit:NOISE:MINimum:FAIL? (segment_number)
CALCulate:LIMit:NOISE:MINimum:FAIL:ALL?
CALCulate:LIMit:SPUR:MAXimum (segment#, start_freq, start_amplitude,
stop_freq, stop_amplitude)
CALCulate:LIMit:SPUR:MAXimum? (segment_number)
CALCulate:LIMit:SPUR:MAXimum:DELETE (segment_number)
CALCulate:LIMit:SPUR:MAXimum:DELETE:ALL
CALCulate:LIMit:SPUR:MAXimum:DISPLAY (0 | OFF | 1 | ON)
CALCulate:LIMit:SPUR:MAXimum:DISPLAY?
CALCulate:LIMit:SPUR:MAXimum:FAIL? (segment_number)
CALCulate:LIMit:SPUR:MAXimum:FAIL:ALL?
CALCulate:LIMit:SPUR:MINimum (segment#, start_freq, start_amplitude,
stop_freq, stop_amplitude)
CALCulate:LIMit:SPUR:MINimum? (segment_number)
CALCulate:LIMit:SPUR:MINimum:DELETE (segment_number)
CALCulate:LIMit:SPUR:MINimum:DELETE:ALL
CALCulate:LIMit:SPUR:MINimum:DISPLAY (0 | OFF | 1 | ON)
CALCulate:LIMit:SPUR:MINimum:DISPLAY?
CALCulate:LIMit:SPUR:MINimum:FAIL? (segment_number)
CALCulate:LIMit:SPUR:MINimum:FAIL:ALL?

```

```
CALCulate:PBWidth  (value)
CALCulate:PBWidth?
CALCulate:SElect  (BOTH | NOISE | SPURs)
CALCulate:SElect?
CALCulate:SMOothing  (value)
CALCulate:SMOothing?
CALCulate:TRANSform  (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
CALCulate:TRANSform?
CALCulate:TVAriance?  (tau, Frequency offset)
CALCulate:VIEW:SPURtable
CALCulate:VIEW:TRACe  (start-offset, stop-offset, #points, distribution
(log/linear))
CALCulate:VIEW:XYData
CALCulate:YShift  (value)
CALCulate:YShift?
```

## CALibrate

```
CALibrate:DETector:CONSTant  (value)
CALibrate:DETector:CONSTant?
CALibrate:DETector:CONSTant:METHod  (BEATnote | DCPeak | SSPur | DSPur |
FMD | AMIN | PShift | NONE)
CALibrate:DETector:CONSTant:METHod?
CALibrate:DETector:CONSTant:SPUR:AMPLitude  (value)
CALibrate:DETector:CONSTant:SPUR:AMPLitude?
CALibrate:DETector:CONSTant:SPUR:OFFSet  (value)
CALibrate:DETector:CONSTant:SPUR:OFFSet?
CALibrate:VCO:IRESistance  (value)
CALibrate:VCO:IRESistance?
CALibrate:VCO:PLLSuppress  (0 | OFF | 1 | ON)
CALibrate:VCO:PLLSuppress?
CALibrate:VCO:PLLSuppress:APOLE?
CALibrate:VCO:PLLSuppress:CBWidth?
CALibrate:VCO:PLLSuppress:PTRange?
CALibrate:VCO:PLLSuppress:DISPLAY[:ALWays]  (0 | OFF | 1 | ON)
CALibrate:VCO:PLLSuppress:DISPLAY[:ALWays]?
CALibrate:VCO:PLLSuppress:ERRor  (value)
CALibrate:VCO:PLLSuppress:ERRor?
CALibrate:VCO:PLLSuppress:ERRor:ACTION  (THEoretical | ADJusted | PAUSE)
CALibrate:VCO:PLLSuppress:ERRor:ACTION?
CALibrate:VCO:TCONSTant:METHod  (CURRent | MEASure | CALCulate)
CALibrate:VCO:TCONSTant:METHod?
CALibrate:VCO:TCONSTant:NOMinal  (value)
CALibrate:VCO:TCONSTant:NOMinal?
CALibrate:VCO:TCONSTant?
CALibrate:VCO:TMODE  (value)
CALibrate:VCO:TMODE?
CALibrate:VCO:VCADjust  (value)
CALibrate:VCO:VCADjust?
CALibrate:VCO:VCENTER  (value)
CALibrate:VCO:VCENTER?
CALibrate:VCO:VRANGE  (value)
CALibrate:VCO:VRANGE?
DISPLAY
DISPLAY:GRAPH:BOUNds:AMPLitude  (Transform,Min,Max)
DISPLAY:GRAPH:BOUNds:AMPLitude?  (SSBN | SDPF | SDFF | SFFF | NF2P | AMN
| BBAN)
```

```

DISPlay:GRAPH:BOUNds:FREQuency (Min,Max)
DISPlay:GRAPH:BOUNds:FREQuency?
DISPlay:GRAPH:CFSCale (value)
DISPlay:GRAPH:CFSCale?
DISPlay:GRAPH:DIPower (value)
DISPlay:GRAPH:DIPower?
DISPlay:GRAPH:PBWidth (value)
DISPlay:GRAPH:PBWidth?
DISPlay:GRAPH:SMOothing (value)
DISPlay:GRAPH:SMOothing?
DISPlay:GRAPH:TRANSform (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
DISPlay:GRAPH:TRANSform?
DISPlay:GRAPH:YShift (value)
DISPlay:GRAPH:YShift?
DISPlay:MEASurement:TIME?
DISPlay:TEXT:TITLe ("string")
DISPlay:TEXT:TITLe?

```

## FORMat

```
FORMat [:DATA] (ASCii | REAL, length)
```

## INITiate

```

INITiate[:IMMEDIATE]:CALibrate
INITiate[:IMMEDIATE]:MEASure
INITiate[:IMMEDIATE][:ALL]

```

## MMEMemory

```

MMEMemory:LOAD [:ALL] ("path\file.pnm")
MMEMemory:STORe [:ALL] ("path\file.pnm")

```

## PAUSe

```

PAUSE:ABORT:AUTO (0 | OFF | 1 | ON)
PAUSE:ABORT:AUTO?
PAUSE:ADJust:VCOCenter (value)
PAUSE:ADJust:VCOCenter?
PAUSE:ADJust:LNAGain (14 | 28 | 42 | 56)
PAUSE:ADJust:LNAGain?
PAUSE:CONNect (0 | OFF | 1 | ON)
PAUSE:CONNect?
PAUSE:CONTinue
PAUSE:RETRY
PAUSE:SPECial

```

## SENSe

```

[:SENSe] :DATA?
[:SENSe] :DATA:HEADER:POINTS?
[:SENSe] :DCONverter:ATTenuator (0 to 35 dB in 5 dB steps)
[:SENSe] :DCONverter:ATTenuator?
[:SENSe] :DCONverter:ATTenuator:AUTO (0 | OFF | 1 | ON)
[:SENSe] :DCONverter:ATTenuator:AUTO?
[:SENSe] :DCONverter:ATTenuator:AUTO:IMMediate
[:SENSe] :DCONverter:BAND (UWAVe | A | K | Q | U | V | W)
[:SENSe] :DCONverter:BAND?
[:SENSe] :DCONverter:FREQuency (value)
[:SENSe] :DCONverter:FREQuency?
[:SENSe] :DCONverter:IFFRequency?
[:SENSe] :DCONverter:IFGain (-10 to 45 dB in 5 dB steps)
[:SENSe] :DCONverter:IFGain?
[:SENSe] :DCONverter:IFGain:AUTO (0 | OFF | 1 | ON)
[:SENSe] :DCONverter:IFGain:AUTO?
[:SENSe] :DCONverter:IFGain:AUTO:IMMediate
[:SENSe] :DCONverter:L1BWidth (value)
[:SENSe] :DCONverter:L1BWidth?
[:SENSe] :DCONverter:L6BWidth (value)
[:SENSe] :DCONverter:L6BWidth?
[:SENSe] :DCONverter:LOPower (value)
[:SENSe] :DCONverter:LOPower?
[:SENSe] :DCONverter:LOSelect (value)
[:SENSe] :DCONverter:LOSelect?
[:SENSe] :DCONverter:LOSelect:AUTO (0 | OFF | 1 | ON)
[:SENSe] :DCONverter:LOSelect:AUTO?
[:SENSe] :DCONverter:MEXT:BIAS (value)
[:SENSe] :DCONverter:MEXT:BIAS?
[:SENSe] :DCONverter:MEXT:BIAS:STATE (0 | OFF | 1 | ON)
[:SENSe] :DCONverter:MEXT:BIAS:STATE?
[:SENSe] :DCONverter:MMLO?
[:SENSe] :DCONverter:PLO
[:SENSe] :DCONverter:REFerence (value)
[:SENSe] :DCONverter:REFerence?
[:SENSe] :DCONverter:TSENsitivity?
[:SENSe] :DCONverter:TUNE:PORT (OFF | INTERNAL | FRONT | REAR)
[:SENSe] :DCONverter:TUNE:PORT?
[:SENSe] :DETEctor:FREQuency (value)
[:SENSe] :DETEctor:FREQuency?
[:SENSe] :DETEctor:SElect (AUTO | EXT | LFR | HFR | UWAVe | TAM | TINoise
| DCAM)
[:SENSe] :DETEctor:SElect?
[:SENSe] :FFT:INPut:COUPling (AC | DC)
[:SENSe] :FFT:INPut:COUPling?
[:SENSe] :NOISE:BBGain (value)
[:SENSe] :NOISE:BBGain?
[:SENSe] :NOISE:FFT (EXTended | MULTiple)
[:SENSe] :NOISE:FFT?
[:SENSe] :NOISE:MEAStype (ABS | RES | FM | AM | BBAN | NOTS)
[:SENSe] :NOISE:MEAStype?
[:SENSe] :NOISE:PULSed (0 | OFF | 1 | ON)
[:SENSe] :NOISE:PULSed?
[:SENSe] :NOISE:QUADrature[:METHOD] (PSHifter | SOURCE)
[:SENSe] :NOISE:QUADrature[:METHOD]?

```

```

[:SENSe] :RANGE:FFT:AVERage:MINimum (value)
[:SENSe] :RANGE:FFT:AVERage:MINimum?
[:SENSe] :RANGE:FFT:SEGTable[:MEASurement] [:QUALity] (NORMal | FAST | HRESolution | CUSTOM)
[:SENSe] :RANGE:FFT:SEGTable[:MEASurement] [:QUALity]?
[:SENSe] :RANGE:OFFSet (Start frequency,Stop frequency)
[:SENSe] :RANGE:OFFSet?
[:SENSe] :RANGE:SWEPt:SEGTable[:MEASurement] [:QUALity] (NORMal | FAST | HRESolution | CUSTOM)
[:SENSe] :RANGE:SWEPt:SEGTable[:MEASurement] [:QUALity]?
[:SENSe] :TSET:ATTenuator (0 to 35 dB in 5 dB steps)
[:SENSe] :TSET:ATTenuator?
[:SENSe] :TSET:ATTenuator:AUTO (0 | OFF | 1 | ON)
[:SENSe] :TSET:ATTenuator:AUTO?
[:SENSe] :TSET:DCBlock (0 | OFF | 1 | ON)
[:SENSe] :TSET:DCBlock?
[:SENSe] :TSET:LNAGain (14 | 28 | 42 | 56)
[:SENSe] :TSET:LNAGain?
[:SENSe] :TSET:LNAGain:METHod (AUTO | FIXED | PAUSE)
[:SENSe] :TSET:LNAGain:METHod?
[:SENSe] :TSET:LNAGain:MINimum (value)
[:SENSe] :TSET:LNAGain:MINimum?
[:SENSe] :TSET:LPF (value)
[:SENSe] :TSET:LPF?
[:SENSe] :TSET:LPF:AUTO (0 | OFF | 1 | ON)
[:SENSe] :TSET:LPF:AUTO?
[:SENSe] :TSET:PLL:ATTenuator (value)
[:SENSe] :TSET:PLL:ATTenuator?
[:SENSe] :TSET:PLL:UNLock:IGNore (0 | OFF | 1 | ON)
[:SENSe] :TSET:PLL:UNLock:IGNore?
[:SENSe] :TVCO (REFerence | CARRier | DCONverter | INTernal)
[:SENSe] :TVCO?
[:SENSe] :TSET:MLEvel:AMDetector (value)
[:SENSe] :TSET:MLEvel:AMDetector?
[:SENSe] :TSET:MLEvel:RFDetector (value)
[:SENSe] :TSET:MLEvel:RFDetector?
[:SENSe] :TSET:MLEvel:UWDetector (value)
[:SENSe] :TSET:MLEvel:UWDetector?
[:SENSe] :VIEW:DCONverter (BBAND | CARRier | IF)
[:SENSe] :VIEW:DCONverter?
[:SENSe] :VIEW:TSET (BBAND | CARRier | IF)
[:SENSe] :VIEW:TSET?

```

## SOUrce

```

SOURce:CALibration:FM:INTernal:FREQuency (value)
SOURce:CALibration:FM:INTernal:FREQuency?
SOURce:CALibration:FM[:DEViation] (value)
SOURce:CALibration:FM[:DEViation]?
SOURce:CALibration:FREQuency[:CW|FIXed] (value)
SOURce:CALibration:FREQuency[:CW|FIXed]?
SOURce:CALibration:POWer[:LEVel|AMPLitude] (value)
SOURce:CALibration:POWer[:LEVel|AMPLitude]?
SOURce:CARRier:FREQuency[:CW|FIXed] (value)
SOURce:CARRier:FREQuency[:CW|FIXed]?

```

```
SOURce:CARRier:POWeR[:LEVel|AMPLitude] (value)
SOURce:CARRier:POWeR[:LEVel|AMPLitude]?
SOURce:REFerence:FREQuency:DIVisor (value)
SOURce:REFerence:FREQuency:DIVisor?
SOURce:REFerence:FREQuency:MULTiplier (value)
SOURce:REFerence:FREQuency:MULTiplier?
SOURce:REFerence:POWeR[:LEVel|AMPLitude] (value)
SOURce:REFerence:POWeR[:LEVel|AMPLitude]?
SOURce:RESidual:FREQuency[:CW|FIXed] (value)
SOURce:RESidual:FREQuency[:CW|FIXed]?
SOURce:RESidual:FREQuency:CALCulate (0 | OFF | 1 | ON)
SOURce:RESidual:FREQuency:CALCulate?
SOURce:RESidual:FREQuency:DIVisor (value)
SOURce:RESidual:FREQuency:DIVisor?
SOURce:RESidual:FREQuency:DETector:COUPled (0 | OFF | 1 | ON)
SOURce:RESidual:FREQuency:DETector:COUPled?
SOURce:RESidual:FREQuency:MULTiplier (value)
SOURce:RESidual:FREQuency:MULTiplier?
SOURce:RESidual:POWeR[:LEVel|AMPLitude] (value)
SOURce:RESidual:POWeR[:LEVel|AMPLitude]?
```

## STATus

```
STATus:ADVise:ENABLE (0 | OFF | 1 | ON)
STATus:ADVise:ENABLE?
STATus:OPERation:CONDITION?
STATus:OPERation:ENABLE (value)
STATus:OPERation:ENABLE?
STATus:OPERation:EVENT?
STATus:OPERation:NTRansition (value)
STATus:OPERation:NTRansition?
STATus:OPERation:PTRansition (value)
STATus:OPERation:PTRansition?
STATus:PRESet
STATus:QUESTIONable:CONDITION?
STATus:QUESTIONable:ENABLE (value)
STATus:QUESTIONable:ENABLE?
STATus:QUESTIONable:EVENT?
STATus:QUESTIONable:NTRansition (value)
STATus:QUESTIONable:NTRansition?
STATus:QUESTIONable:PTRansition (value)
STATus:QUESTIONable:PTRansition?
```

## SYSTem

```
SYSTem:ASSET:CALSource ("None" | "asset_name")
SYSTem:ASSET:CALSource?
SYSTem:ASSET:CARRier ("None" | "asset_name")
SYSTem:ASSET:CARRier?
SYSTem:ASSET:COUNTER ("None" | "asset_name")
SYSTem:ASSET:COUNTER?
SYSTem:ASSET:DCONverter ("None" | "asset_name")
SYSTem:ASSET:DCONverter?
SYSTem:ASSET:DCONverter:USAGE (NONE | MANUAL | SYSTem)
SYSTem:ASSET:DCONverter:USAGE?
```

```
SYSTem:ASSet:FFT  ("None" | "asset_name")
SYSTem:ASSet:FFT?
SYSTem:ASSet:FFT:CUSTom[:SEGTable]  ("path\name.fst")
SYSTem:ASSet:PSHifter  ("None" | "asset_name")
SYSTem:ASSet:PSHifter?
SYSTem:ASSet:REFerence  ("None" | "asset_name")
SYSTem:ASSet:REFerence?
SYSTem:ASSet:RESidual  ("None" | "asset_name")
SYSTem:ASSet:RESidual?
SYSTem:ASSet:SLAVe:SOURce  ("None" | "asset_name")
SYSTem:ASSet:SLAVe:SOURce?
SYSTem:ASSet:SLAVe:SOURce:PORT  (LOINput | AUXinput)
SYSTem:ASSet:SLAVe:SOURce:PORT?
SYSTem:ASSet:SWANalyzer  ("None" | "asset_name")
SYSTem:ASSet:SWANalyzer?
SYSTem:ASSet:SWANalyzer:CUSTom[:SEGTable]  ("path\name.sst")
SYSTem:ASSet:TBASe  ("None" | "asset_name")
SYSTem:ASSet:TBASe?
SYSTem:ASSet:TSET  ("None" | "asset_name")
SYSTem:ASSet:TSET?
SYSTem:ERror?
SYSTem:GUI:LLOCKout
SYSTem:GUI:REMote  (0 | OFF | 1 | ON)
SYSTem:GUI:REMote?
SYSTem:HELP:HEADers?
SYSTem:PATH:CARRier  (TSET | DCONverter)
SYSTem:PATH:CARRier?
SYSTem:PATH:DCBBanalyzer  (TSLF | TSHF | TSRF)
SYSTem:PATH:DCBBanalyzer?
SYSTem:PATH:FFTAnalyzer  (TSLF | TSHF | TSRF | DCRF)
SYSTem:PATH:FFTAnalyzer?
SYSTem:PATH:SWANalyzer  (TSLF | TSHF | TSRF | DCRF)
SYSTem:PATH:SWANalyzer?
SYSTem:PATH:TVCO  (FPANel | RPANel | INTernal)
SYSTem:PATH:TVCO?
SYSTem:VERSION?
```



## 5 Required Commands

- Required Commands Introduction 78
- \*CLS 79
- \*ESE 80
- \*ESR? 81
- \*IDN? 82
- \*OPC 83
- \*OPC? 84
- \*RST 85
- \*SRE 89
- \*STB? 90
- \*TST? 91
- \*WAI 92



## Required Commands Introduction

The following IEEE 488.2 Required Commands are supported:

- \*CLS
- \*ESE (Value)
- \*ESE?
- \*ESR?
- \*IDN?
- \*OPC
- \*OPC?
- \*RST
- \*SRE (Value)
- \*SRE?
- \*STB?
- \*TST?
- \*WAI

## \*CLS

Clears the Status Byte by emptying the error queue and clearing all event registers.

### Command syntax

\*CLS

### Query syntax

Command Only

### Attribute summary

Synchronization Required: no

Preset (\*RST) State: NA

SCPI Compliance: standard

### Additional information

Also see STATus:PRESet command

## **\*ESE**

Specifies which bits in the Event Register (ESR?) set the ESR summary Bit (bit 5) in the Status Byte (\*STB?).

### **Command syntax**

`*ESE (0-255)`

### **Example**

`*ESE 1`

### **Query syntax**

`*ESE?`

### **Attribute summary**

Synchronization Required: no

Preset (\*RST) State: NA

SCPI Compliance: standard

### **Additional information**

See \*ESR for bit assignments.

## \*ESR?

Reads and clears the Standard Event Enable register.

### Command syntax

Query Only

### Query syntax

\*ESR?

### Return format

Integer (0-255)

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: standard

### Additional information

- bit 0 = 1 = Operation Complete
- bit 1 = 2 = Request Control
- bit 2 = 4 = Query Error
- bit 3 = 8 = Device Dependent Error. (Pause, Abort, or Warning, Summary of QSR bits 9,10,11)
- bit 4 = 16 = Execution Error. (synchronous error)
- bit 5 = 32 = Command Error
- bit 6 = 64 = User Request
- bit 7 = 128 = Power On

## **\*IDN?**

Returns a comma-separated list of arbitrary ASCII response data items that uniquely identifies the system.

### **Command syntax**

Query Only

### **Example**

E5500, Phase Noise Measurement Sub system, Version A.01.00

### **Query syntax**

\*IDN?

### **Return format**

ARB\_ASCII

### **Attribute summary**

Synchronization Required: no

Preset (\*RST) State: instrument specific

SCPI Compliance: standard

## \*OPC

Causes bit #0 (Operation Complete) of the Event Status Register to be set to 1 when all pending operations are complete.

### Command syntax

\*OPC

### Query syntax

\*OPC?

### Return format

Integer

### Attribute summary

Synchronization Required: no

Preset (\*RST) State: NA

SCPI Compliance: standard

### Additional information

These are the only commands to which \*OPC, \*OPC? and \*WAI apply:

- INITiate:CALibrate
- INITiate:MEASure
- INITiate:IMMediate:ALL

All other commands execute immediately and do not cause pending operations.

## **\*OPC?**

Returns a ASCII 1 when all pending operations are complete.

### **Command Syntax**

Query Only

### **Query syntax**

OPC?

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: no

Preset (\*RST) State: NA

SCPI Compliance: standard

### **Additional information**

These are the only commands to which \*OPC, \*OPC? and \*WAI apply:

- INITiate:CALibrate
- INITiate:MEASure
- INITiate:IMMEDIATE:ALL

All other commands execute immediately and do not cause pending operations.

## \*RST

Executes a device reset.

### Command syntax

\*RST

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: standard

### Additional information

After \*RST parameter queries return the following values:

- CALCulate:CFSCale? 1.00000000
- CALCulate:DATA:HEADER:POINTs? +0
- CALCulate:DIPower? 0.00000000
- CALCulate:PBWidth? 1.00000000
- CALCulate:SELect? BOTH
- CALCulate:SMOothing? +0
- CALCulate:TRANSform? SSBNoise
- CALCulate:YShift? 0.00000000
- CALibrate:DETEctor:CONSTant:METHod? BEATnote
- CALibrate:DETEctor:CONSTant:SPUR:AMPLitude? -130.00000000
- CALibrate:DETEctor:CONSTant:SPUR:OFFSet? 1.00000000
- CALibrate:DETEctor:CONSTant? 1.00000000E-6
- CALibrate:VCO:IRESistance? 1.00000000E+06
- CALibrate:VCO:PLLSuppress:DISPLAY:ALWays? 0
- CALibrate:VCO:PLLSuppress:ERRor:ACTion? ADJusted
- CALibrate:VCO:PLLSuppress:ERRor? 1.00000000
- CALibrate:VCO:PLLSuppress? 1

## 5 Required Commands

- CALibrate:VCO:TCONstant:METHod? MEASure
- CALibrate:VCO:TCONstant:NOMinal? 10.00000000E+03
- CALibrate:VCO:TCONstant? 1.00000000E+06
- CALibrate:VCO:TMODe? EFC
- CALibrate:VCO:VCADjust? 1.00000000
- CALibrate:VCO:VCENter? 0.00000000
- CALibrate:VCO:VRANge? 1.00000000
- DISPlay:GRAPH:BOUNds:AMPLitude? SSBN -170.00000000, 0.00000000
- DISPlay:GRAPH:BOUNds:AMPLitude? SDPF -170.00000000, 0.00000000
- DISPlay:GRAPH:BOUNds:AMPLitude? SDFF 1.00000000E-6,  
1.00000000E+03
- DISPlay:GRAPH:BOUNds:AMPLitude? SFFF 1.00000000E-15,  
1.00000000E-6
- DISPlay:GRAPH:BOUNds:AMPLitude? NF2P -170.00000000, 0.00000000
- DISPlay:GRAPH:BOUNds:AMPLitude? AMN -170.00000000, 0.00000000
- DISPlay:GRAPH:BOUNds:AMPLitude? BBAN -170.00000000, 0.00000000
- DISPlay:GRAPH:BOUNds:FREQuency? 1.00000000, 100.00000000E+06
- DISPlay:GRAPH:CFSCale? 1.00000000
- DISPlay:GRAPH:DIPower? 0.00000000
- DISPlay:GRAPH:PBWidth? 1.00000000
- DISPlay:GRAPH:SMOothing? +0
- DISPlay:GRAPH:TRANSform? SSBNoise
- DISPlay:GRAPH:YShift? 0.00000000
- DISPlay:TEXT:TITLE? E5500 Absolute Phase Noise Measurement
- FORMat:DATA? ASCii,6
- PAUSe:ABORt:AUTO? 1
- PAUSe:CONNect? 0
- SOURce:CALibration:FM:INTERNAL:FREQuency? 1.00000000E+03
- SOURce:CALibration:FM:DEViation? 10.00000000E+03
- SOURce:CALibration:FREQuency:FIXed? 500.00000000E+06
- SOURce:CALibration:POWer:AMPLitude? 10.00000000
- SOURce:CARRier:FREQuency:FIXed? 500.00000000E+06
- SOURce:CARRier:POWer:AMPLitude? 10.00000000
- SOURce:REFerence:POWer:AMPLitude? 10.00000000
- SOURce:RESidual:FREQuency:FIXed? 500.00000000E+06

- SOURce:RESidual:POWer:AMPLitude? 10.00000000
- STATus:ADVise:ENABLE? 0
- SYSTem:ASSet:DCONverter:USAGe? NONE
- SYSTem:ASSet:SLAve:SOURce:PORT? LOINput
- SYSTem:PATH:CARRier? TSET
- SYSTem:PATH:DCBBanalyzer? TSLF
- SYSTem:PATH:FFTAnalyzer? TSLF
- SYSTem:PATH:SWANalyzer? TSLF
- SYSTem:PATH:TVCO? FPANel
- SENSe:DATA:HEAdEr:POINts? +0
- SENSe:DCONverter:ATTenuator:AUTO? 1
- SENSe:DCONverter:ATTenuator? 0.00000000
- SENSe:DCONverter:BAND? UWAVe
- SENSe:DCONverter:FREQuency? 10.0000000E+09
- SENSe:DCONverter:IFFRrequency? 0.00000000
- SENSe:DCONverter:IFGain:AUTO? 1
- SENSe:DCONverter:IFGain? 0.00000000
- SENSe:DCONverter:L1BWidth? 126
- SENSe:DCONverter:L6BWidth? 10e3
- SENSe:DCONverter:LOPower? 10.00000000
- SENSe:DCONverter:LOSelect:AUTO? 1
- SENSe:DCONverter:LOSelect? 1.00000000E+09
- SENSe:DCONverter:MEXT:BIAS:STATE? 0
- SENSe:DCONverter:MEXT:BIAS? 0.00000000
- SENSe:DCONverter:MLEVel:AMDetector? 0.00000000
- SENSe:DCONverter:MLEVel:UWMixer? 0.00000000
- SENSe:DCONverter:MMLO? 0.00000000
- SENSe:DCONverter:REFERence? 10e+6
- SENSe:DCONverter:TSENsitivity? 0
- SENSe:DCONverter:TUNE:PORT? 0
- SENSe:DETector:FREQuency? 500.00000000E+06
- SENSe:DETector:SElect? AUTO
- SENSe:FFT:INPut:COUpling? AC
- SENSe:NOISe:BBGain? 0.00000000
- SENSe:NOISe:FFT? MULTiple

## 5 Required Commands

- SENSe:NOISe:MEAStype? ABSolute
- SENSe:NOISe:PULSed? 0
- SENSe:NOISe:QUADrature:METHod? SOURce
- SENSe:RANGE:FFT:AVERage:MINimum? +4
- SENSe:RANGE:FFT:SEGTable:MEASurement:QUALity? NORMAl
- SENSe:RANGE:OFFSet? 1.0000000, 100.0000000E+06
- SENSe:RANGE:SWEPt:SEGTable:MEASurement:QUALity?NORMAl
- SENSe:TSET:ATTenuator:AUTO? 1
- SENSe:TSET:ATTenuator? 0
- SENSe:TSET:DCBlock? 0
- SENSe:TSET:LNAGain:METHod? AUTO
- SENSe:TSET:LNAGain:MINimum? 14
- SENSe:TSET:LNAGain? 42
- SENSe:TSET:LPF:AUTO? 1
- SENSe:TSET:LPF? 20e+3
- SENSe:TSET:MLEVel:AMDetector? 0.00000000
- SENSe:TSET:MLEVel:RFDetector? 0.00000000
- SENSe:TSET:MLEVel:UWDetector? 0.00000000
- SENSe:TSET:PLL:ATTenuator? 0.0
- SENSe:TSET:PLL:UNLock:IGNore? 0
- SENSe:TVCO? REference
- SENSe:VIEW:DCONverter? BBAND
- SENSe:VIEW:TSET? BBAND

## \*SRE

Specify bits in the Service Request Enable register (masks status byte).

### Command syntax

```
*SRE <number>
<number> ::= an integer (NRF data)
              limits: 0:191
```

### Example

```
*SRE 32
```

### Query syntax

```
*SRE?
```

### Return format

Integer 0-191

### Attribute summary

Synchronization Required: none

Preset (\*RST) State:NA

SCPI Compliance: standard

### Additional information

Enabled bits will cause and SRQ to be issued and bit 6 (RQS) of the Status Byte to be set. Valid range is 0-191 as \*SRE bit 6 (value 64) can not be set. See \*STB for bit assignments.

## **\*STB?**

Reads the Status Byte register

### **Command syntax**

Query Only

### **Query syntax**

\*STB?

### **Return format**

Integer 0-255

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: IEEE 488.2

### **Additional information**

- bit 0 = 1 = Not Used
- bit 1 = 2 = Not Used
- bit 2 = 4 = Device Dependent Warning, Pause, Error Message Available
- bit 3 = 8 = Summary of Questionable Status Register
- bit 4 = 16 = Message Available (MAV)
- bit 5 = 32 = Summary of Standard Event Status Register
- bit 6 = 64 = Request Service (RQS)
- bit 7 = 128 = Summary of Operation Status Register

## \*TST?

Performs system self test.

### Command syntax

Query Only

### Query syntax

\*TST?

### Return format

Integer

- 0 = Passed Self Test
- non 0 = Failed Self Test

### Attribute summary

Synchronization Required: none

Preset (\*RST) State:NA

SCPI Compliance:IEEE 488.2

### Additional information

Failure messages are placed in the error queue read by SYSTem:ERRor?

## **\*WAI**

Holds off processing of subsequent commands until all preceding commands have been processed.

### **Command syntax**

`*WAI`

### **Query syntax**

Command Only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: standard

### **Additional information**

These are the only commands to which \*OPC, \*OPC? and \*WAI apply:

- INITiate:CALibrate
- INITiate:MEASure
- INITiate:IMMediate:ALL

All other commands execute immediately and do not cause pending operations.

## 6 **ABORt Commands**

ABORt 94



**Agilent Technologies**

## **ABORt**

Terminates any measurement, calibration or pause point and causes the system to return to its idle state without changing any measurement definition parameters.

### **Command syntax**

ABORT

### **Example**

ABORT

### **Query syntax**

Command only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: standard

## 7

# CALCulate Commands

- CALCulate Commands Introduction 97
- CALCulate:ACCumulated[PHASe]? 99
- CALCulate:AVARiance? 100
- CALCulate:CFScale 101
- CALCulate:DATA? 102
- CALCulate:DATA:HEADER:POINTs? 104
- CALCulate:DIPower 105
- CALCulate:F20Scillator[:COMParE] 106
- CALCulate:F30Scillator[:COMParE] 108
- CALCulate:INTEGRal? 110
- CALCulate:INTEGRal:TYPE 111
- CALCulate:LIMit:NOISE:MAXimum 112
- CALCulate:LIMit:NOISE:MAXimum:DElete 113
- CALCulate:LIMit:NOISE:MAXimum: DElete:ALL 114
- CALCulate:LIMit:NOISE:MAXimum:DISPlay 115
- CALCulate:LIMit:NOISE:MAXimum:FAIL? 116
- CALCulate:LIMit:NOISE:MAXimum:FAIL: ALL? 117
- CALCulate:LIMit:NOISE:MINimum 118
- CALCulate:LIMit:NOISE:MINimum:DElete 119
- CALCulate:LIMit:NOISE:MINimum: DElete:ALL 120
- CALCulate:LIMit:NOISE:MINimum:DISPlay 121
- CALCulate:LIMit:NOISE:MINimum:FAIL? 122
- CALCulate:LIMit:NOISE:MINimum: FAIL:ALL? 123
- CALCulate:LIMit:SPUR:MAXimum 124
- CALCulate:LIMit:SPUR:MAXimum:DElete 125
- CALCulate:LIMit:SPUR:MAXimum: DElete:ALL 126
- CALCulate:LIMit:SPUR:MAXimum:DISPlay 127
- CALCulate:LIMit:SPUR:MAXimum:FAIL? 128
- CALCulate:LIMit:SPUR:MAXimum: FAIL:ALL? 129
- CALCulate:LIMit:SPUR:MINimum 130
- CALCulate:LIMit:SPUR:MINimum:DElete 131
- CALCulate:LIMit:SPUR:MINimum: DElete:ALL 132
- CALCulate:LIMit:NOISE:MINimum:DISPlay 133
- CALCulate:LIMit:SPUR:MINimum:FAIL? 134



## **7 CALCulate Commands**

CALCulate:LIMit:SPUR:MINimum: FAIL:ALL? 135

CALCulate:PBWidth 136

CALCulate:SElect 137

CALCulate:SMOothing 138

CALCulate:TVARiance? 140

CALCulate:VIEW:SPURtable 141

CALCulate:VIEW:TRACe 142

CALCulate:VIEW:XYData 143

CALCulate:YShift 144

## CALCulate Commands Introduction

Use the CALCulate commands to perform post acquisition data processing.

The commands in this subsystem have the following command hierarchy:

- CALCulate:ACCumulated[:PHASe]? (tau, start-offset, stop-offset)
- CALCulate:AVARiance? (tau, Frequency offset)
- CALCulate:CFSCale (value)
- CALCulate:CFSCale?
- CALCulate:DATA?
- CALCulate:DATA:HEADER:POINTS?
- CALCulate:DIPower (value)
- CALCulate:DIPower?
- CALCulate:F2OScillator[:COMPARE] ("inFileA", "inFileAB", "outFile"[,"title"])
- CALCulate:F3OScillator[:COMPARE] ("inFileAB", "inFileAC", "inFileBC", "outFileA", "outFileB", "outFileC"[,"titleA", "titleB", "titleC"])
- CALCulate:INTEGRal?
- CALCulate:INTEGRal:TYPE
- CALCulate:LIMit:NOISE:MAXimum (segment#, start\_freq, start\_amplitude, stop\_freq, stop\_amplitude)
- CALCulate:LIMit:NOISE:MAXimum:DElete (segment\_number)
- CALCulate:LIMit:NOISE:MAXimum:DElete:ALL
- CALCulate:LIMit:NOISE:MAXimum:DISPLAY (0 | OFF | 1 | ON)
- CALCulate:LIMit:NOISE:MAXimum:DISPLAY?
- CALCulate:LIMit:NOISE:MAXimum:FAIL? (segment\_number)
- CALCulate:LIMit:NOISE:MAXimum:FAIL:ALL?
- CALCulate:LIMit:NOISE:MAXimum? (segment\_number)
- CALCulate:LIMit:NOISE:MINimum (segment#, start\_freq, start\_amplitude, stop\_freq, stop\_amplitude)
- CALCulate:LIMit:NOISE:MINimum? (segment\_number)
- CALCulate:LIMit:NOISE:MINimum:DElete (segment\_number)
- CALCulate:LIMit:NOISE:MINimum:DElete:ALL
- CALCulate:LIMit:NOISE:MINimum:DISPLAY (0 | OFF | 1 | ON)
- CALCulate:LIMit:NOISE:MINimum:DISPLAY?
- CALCulate:LIMit:NOISE:MINimum:FAIL? (segment\_number)
- CALCulate:LIMit:NOISE:MINimum:FAIL:ALL?

- CALCulate:LIMit:SPUR:MAXimum (segment#, start\_freq, start\_amplitude, stop\_freq, stop\_amplitude)
- CALCulate:LIMit:SPUR:MAXimum? (segment\_number)
- CALCulate:LIMit:SPUR:MAXimum:DElete (segment\_number)
- CALCulate:LIMit:SPUR:MAXimum:DElete:ALL
- CALCulate:LIMit:SPUR:MAXimum:DISPlay (0 | OFF | 1 | ON)
- CALCulate:LIMit:SPUR:MAXimum:DISPlay?
- CALCulate:LIMit:SPUR:MAXimum:FAIL? (segment\_number)
- CALCulate:LIMit:SPUR:MAXimum:FAIL:ALL?
- CALCulate:LIMit:SPUR:MINimum (segment#, start\_freq, start\_amplitude, stop\_freq, stop\_amplitude)
- CALCulate:LIMit:SPUR:MINimum:DElete (segment\_number)
- CALCulate:LIMit:SPUR:MINimum:DElete:ALL
- CALCulate:LIMit:SPUR:MINimum:DISPlay (0 | OFF | 1 | ON)
- CALCulate:LIMit:SPUR:MINimum:DISPlay?
- CALCulate:LIMit:SPUR:MINimum:FAIL? (segment\_number)
- CALCulate:LIMit:SPUR:MINimum:FAIL:ALL?
- CALCulate:LIMit:SPUR:MINimum? (segment\_number)
- CALCulate:PBWidth (value)
- CALCulate:PBWidth?
- CALCulate:SElect (BOTH | NOISe | SPURs)
- CALCulate:SElect?
- CALCulate:SMOothing (value)
- CALCulate:SMOothing?
- CALCulate:TRANSform (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
- CALCulate:TRANSform?
- CALCulate:TVARIance? (tau, Frequency offset)
- CALCulate:VIEW:SPURtable
- CALCulate:VIEW:TRACe (start-offset, stop-offset, #points, distribution (log/linear))
- CALCulate:VIEW:XYData
- CALCulate:YShift (value)
- CALCulate:YShift?

## CALCulate:ACCumulated[PHASe]?

Accumulated phase noise integration.

### NOTE

This optional command requires users to purchase a license to use. If the user attempts to use the command without a license, an error message is generated in the SYST:ERR? queue.

### Command Syntax

Query Only

### Query syntax

```
CALCulate:Accumulated? <tau>,<offset upper value>,
<stop offset>
```

### Example

```
CALCulate:Accumulated? 1,100,100E9
```

### Return format

Real

### Attribute summary

Synchronization Required:none

Preset (\*RST) State: NA

SCPI Compliance:Instrument Specific.

### Additional information

Performs calculation on currently selected data as specified by CALCULATE:SElect (BOTH|NOISE|SPURs)

## CALCulate:AVARiance?

Allan Variance calculation.

### Command Syntax

Query Only

### Query syntax

```
CALCulate:AVARiance? <tau>,<offset upper value>
```

### Example

```
CALCulate:AVARiance? 1,10E3
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

### Additional information

Performs calculation on currently selected data as specified by  
CALCulate:SElect (BOTH|NOISE|SPURs)

## CALCulate:CFSCale

Carrier frequency scale multiplier.

### Command syntax

```
CALCulate:CFSCale <number>
<number> ::= a real number (NRf data)
```

### Example

```
CALCulate:CFSCale 2
```

### Query syntax

```
CALCulate:CFSCale?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1.0

SCPI Compliance:Instrument Specific.

### Additional information

Applied to data output by CALCulate:DATA? when outputting:

- CALCulate:VIEW:TRACe (start, stop, #points, distribute (log/linear) or
- CALCulate:VIEW:XYData.

## CALCulate:DATA?

Provides access to measurement data as processed by the CALCulate subsystem.

### Command syntax

Query Only

### Query syntax

CALCulate:DATA?

### Return format

Varies with CALCulate:VIEW. See Additional information below. Frequencies and Amplitudes are Reals. Spurs and Flags are integers.

### Attribute summary

Synchronization Required: none

Preset (\*RST) State:

- CALCulate:VIEW:XYData
- CALCulate:CFSCale 0
- CALCulate:DIPower 0
- CALCulate:PBWidth 1
- CALCulate:SElect BOTH
- CALCulate:SMOothing 0
- CALCulate:TRANSform SSBN
- CALCulate:YShift 0

SCPI Compliance: Instrument Specific.

### Additional information

Returns a one line per data point as indicated by CALCulate:DATA:HEADER:POINTs. Data type returned is last sent CALCulate:VIEW command which in turn is affected by the current setting of the commands listed under each CALCulate:VIEW command below. The number of significant digits for frequency and amplitude is controlled by the FORMat[:DATA] command.

- CALCulate:VIEW:SPURtable returns “frequency, amplitude” per point.

- CALCulate:TRANSform (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
- CALCulate:YShift (value)
- CALCulate:VIEW:TRACe (start, stop, #points, distribution (log/linear)) returns “amplitude” per point.
  - CALCulate:CFSCale (value)
  - CALCulate:DIPower (value)
  - CALCulate:PBWidth (value)
  - CALCulate:SElect (BOTH | NOISe | SPURs)
  - CALCulate:SMOothing (value)
- CALCulate:TRANSform (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
- CALCulate:YShift (value)
- CALCulate:VIEW:XYData returns “frequency, Amplitude, spur\_flag (1=spur 0=noise)” per point.
  - CALCulate:CFSCale (value)
  - CALCulate:DIPower (value)
  - CALCulate:PBWidth (value)
  - CALCulate:SElect (BOTH | NOISe | SPURs)
  - CALCulate:SMOothing (value)
- CALCulate:TRANSform (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
- CALCulate:YShift (value)

## CALCulate:DATA:HEADer:POINts?

Returns the number of data points which will be returned by CALCule:DATA?

### Command Syntax

Query Only

#### Query syntax

```
CALCulate:DATA:HEADer:POINTS?
```

#### Example

```
CALCulate:DATA:HEADer:POINTS?
```

#### Return format

Integer

#### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Instrument Specific.

## CALCulate:DIPower

DUT input power adjustment.

### Command syntax

```
CALCulate:DIPower <number>
<number> ::= a real number (NRf data)
```

### Example

```
CALCulate:DIPower -10
```

### Query syntax

```
CALCulate:DIPower?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0.0

SCPI Compliance: Instrument Specific.

### Additional information

Applied to data output by CALCulate:DATA? when outputting:

CALCulate:VIEW:TRACe (start, stop, #points, distribution (log/linear)) or  
CALCulate:VIEW:XYData

## **CALCulate:F2OScillator[:COMPARE]**

Function compares 2 oscillator measurement files and outputs a new measurement file of the result.

### **Command syntax**

```
CALCulate:F2OScillator[:COMPARE] <"InFileA.pnm", "InFileAB.pnm",
"OutFileB.pnm" [, "Title"]>
" InFileA.pnm" ::= Input file of DUT A oscillator measurement from the
result of a previous 3 Oscillator comparison.
" InFileAB.pnm" ::= Input file of DUT A vs DUT B oscillator measurement.
" OutFileB.pnm" ::= Output file of calculated DUT B oscillator. File names
are quoted strings (full or relative path and filename).
" Title" ::= Optional quoted string title for graph displayed by output
file. Defaults to file name of output file.
```

### **Example**

```
CALCulate:F2OScillator "Ref.pnm", "RefvsDut.pnm", "Dut.pnm", "2 Osc Result"
```

### **Query syntax**

Command Only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

Input files must exist. Input files must have identical segment tables and measurement ranges.

Note that there is no format specification for files. The files are in a format relevant only to the Phase Noise GUI or SCPI clients (.pnm files)

The 2 Oscillator Comparison determines the actual noise level of the unit under test (UUT) by subtracting the known noise level of the reference source device. This procedure is almost identical to the 3 Oscillator Comparison, except that only one measurement from a pair of devices is necessary.

The 3 Oscillator Comparison must first be done to determine the noise level of the reference device. See CALCulate:F3OScillator[:COMPARE]. Once a known reference level is established, the software subtracts the reference noise from the measurement results. The 2 Oscillator Comparison is valid only if the

Measurement Definition parameters and the segment table parameters are kept the same for the Reference device versus the DUT noise measurement as they were when the Reference device was measured using the 3 Oscillator Comparison.

### **Measurement Uncertainty**

To insure accurate results, the noise levels of the three devices should be within 3 to 6 dB of each other at the frequency offsets of interest. Computation uncertainty increases when the phase noise differs by more than 3 dB between the three devices. A minimum of 20 averages, defined in the Type/Range tab of Measurement Definition menu, is recommended when making the noise measurements.

### **Considerations for the 2 Oscillator Comparison**

Unmarked spurs can cause erroneous results for the 2 Oscillator Comparison. Marked spurs are automatically stripped out during the computation, unmarked spurs are not. Unmarked spurs prevent the test system from performing a proper subtraction since spurs cannot be subtracted on a power basis. Observe the measurement results to insure that a minimum of unmarked spurs are present around the offsets of interest. The number of unmarked spurs within the measurement can be reduced by either reducing the measurement bandwidth, or by increasing the number of averages specified in the Type/Range section of Measurement Definition menu and in the FFT and Swept Segment tables.

## **CALCulate:F30Scillator[:COMPARE]**

Function compares 3 oscillator measurement files and outputs 3 new measurement files of the results.

### **Command syntax**

```
CALCulate:F30Scillator[:COMPARE] <"InFileAB.pnm", "InFileAC.pnm",
" InFileBC.pnm", "OutFileA.pnm", "OutFileB.pnm", "OutFileC.pnm" [, "Title
A", "Title B" "Title C"]>

"InFileAB.pnm" ::= Input file of DUT A vs DUT B oscillator measurement.
"InFileAC.pnm" ::= Input file of DUT A vs DUT C oscillator measurement.
"InFileAC.pnm" ::= Input file of DUT B vs DUT C oscillator measurement.
"OutFileA.pnm" ::= Output file of calculated DUT A oscillator.
"OutFileB.pnm" ::= Output file of calculated DUT B oscillator.
"OutFileC.pnm" ::= Output file of calculated DUT C oscillator.

File names are quoted strings (full or relative path and filename).

"Title (ABC)" ::= Optional quoted string titles for graphs displayed by
output files. Defaults to file name of corresponding output file.
```

### **Example**

```
CALCulate:F30Scillator "DutAvsDutB.pnm", "DutAvsDutC.pnm",
"DutBvsDutC.pnm", "DutA.pnm", "DutB.pnm", "DutC.pnm" "Oscillator A",
"Oscillator B", "Oscillator C"
```

### **Query syntax**

Command Only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

Input files must exist. Input files must have identical segment tables and measurement ranges.

Note that there is no format specification for files. The files are in a format relevant only to the Phase Noise GUI or SCPI clients (.pnm files)

The 3 Oscillator Comparison determines the noise level for each of three similar sources or devices. This comparison is useful when a reference source with a known lower noise level is not available for a direct comparison and is

the only practical way to determine the exact noise level of state-of-the-art sources. The 3 Oscillator Comparison computes the noise level of three separate devices by measuring them in pairs (A vs. B, A vs. C, and then B vs. C). To achieve accurate results, each of the three measurements must be performed under the same conditions (frequency, measurement range, and segment definition). The test system computes the noise level of each device by comparing and analyzing the measurement results for each of the three noise measurements. The SOFTWARE stores the computed noise level for each of the three devices in separate Result (.pnm) files. The following expressions are used to evaluate the three devices:

- A vs. B = XX = The results of device A vs. B without spurs
- A vs. C = YY = The results of device A vs. C without spurs
- B vs. C = ZZ = The results of device B vs. C without spurs

Therefore:

- A =  $(X + Y - Z)/2A$  = The results of device A only
- B =  $(X + Z - Y)/2B$  = The results of device B only
- C =  $(Y + Z - X)/2C$  = The results of device C only

### **Measurement Uncertainty**

To insure accurate results, the noise levels of the three devices should be within 3 to 6 dB of each other at the frequency offsets of interest. Computation uncertainty increases when the phase noise differs by more than 3 dB between the three devices. A minimum of 20 averages, defined in the Type/Range tab of Measurement Definition menu, is recommended when making the noise measurements. A good test to use for verifying the validity of the noise measurements before performing the 3 Oscillator Comparison is to check that the combined level of the two lowest measurements is greater than or equal to the level of the highest measurement

### **Considerations for the 3 Oscillator Comparison**

Unmarked spurs can cause erroneous results for the 3 Oscillator Comparison. Marked spurs are automatically stripped out during the computation, unmarked spurs are not. Unmarked spurs prevent the test system from performing a proper subtraction since spurs cannot be subtracted on a power basis. Observe the measurement results to insure that a minimum of unmarked spurs are present around the offsets of interest. The number of unmarked spurs within the measurement can be reduced by either reducing the measurement bandwidth, or by increasing the number of averages specified in the Type/Range section of Measurement Definition menu and in the FFT and Swept Segment tables.

## CALCulate:INTegral?

Trace integration.

### Command Syntax

Query Only

#### Query syntax

```
CALCulate:INTegral? <start_offset> [<frequency_suffix>],  
                      <stop_offset> [<frequency_suffix>]  
<start_offset>      ::= a real number (NRF data)  
<stop_offset>       ::= a real number (NRF data)  
<frequency_suffix> ::= Hz|kHz|MHz|GHz
```

#### Example

```
CALCulate:INTegral? 10,100E3
```

#### Return format

Real

#### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific

#### Additional information

Performs calculation on currently selected data as specified by:

- CALCulate:SELect (BOTH | NOISe | SPURs)
- CALCulate:TRANSform (SSBN | SDPF | SDFF | SFff | NF2P | AMN | BBAN)

## CALCulate:INTEGRAL:TYPE

Specify the type of integral calculation used by the CALCulate:INTEGRAL command.

NORMAl:

CCITt:

### Command Syntax

```
CALCulate:INTEGRAL:TYPE NORMAl|CCITt
```

### Example

```
CALCulate:INTEGRAL:TYPE CCITt
```

### Query syntax

```
CALCulate:INTEGRAL:TYPE?
```

### Return format

string

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NORMAl

SCPI Compliance: Instrument Specific

### Additional information

When type is set to CCITt, the weighting over frequency is as specified in ITU-T Recommendation 0.41 (10/94), Table 1/0.41.

## CALCulate:LIMit:NOISe:MAXimum

Specifies a limit line segment for the maximum amplitude limit for noise data.

<b>Command syntax</b>	<code>CALCulate:LIMit:NOISe:MAXimum &lt;segment_number&gt;, &lt;start_offset&gt; [&lt;frequency_suffix&gt;], &lt;start_power&gt; [&lt;power_suffix&gt;], &lt;stop_offset&gt; [&lt;frequency_suffix&gt;], &lt;stop_power&gt; [&lt;power_suffix&gt;]</code> <code>&lt;segment_number&gt; ::= an integer in the range 1-100</code> <code>&lt;start_offset&gt; ::= a real number (NRF data)</code> <code>&lt;start_power&gt; ::= a real number (NRF data)</code> <code>&lt;stop_offset&gt; ::= a real number (NRF data)</code> <code>&lt;stop_power&gt; ::= a real number (NRF data)</code>
-----------------------	--

### Example

```
CALC:LIMit:NOISe:MAX 1, 100, -50, 10e3, -80
```

### Query syntax

```
CALCulate:LIMit:NOISe:MAXimum? <segment_number>
CALC:LIMit:NOISe:MAX? 1
```

### Return format

Real, Real, Real, Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: (all segments deleted)

SCPI Compliance: Instrument Specific.

### Additional information

Segment amplitude units are those of the current display graph type.

## CALCulate:LIMit:NOISe:MAXimum:DELete

Delete the specified limit line segment for the maximum amplitude limit for noise data.

### Command syntax

```
CALCulate:LIMit:NOISe:MAXimum:DELETE <segment_number>
<segment_number> ::= an integer in the range 1-100
```

### Example

```
CALC:LIMit:NOISe:MAX:DElete 1
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## **CALCulate:LIMIT:NOISE:MAXimum: DElete:ALL**

Delete all limit line segments for the maximum amplitude limit for noise data.

### **Command syntax**

`CALCulate:LIMIT:NOISE:MAXimum:DElete:ALL`

### **Example**

`CALC:LIMIT:NOISE:MAX:DElete:ALL`

### **Query syntax**

Command Only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:NOISe:MAXimum:DISPlay

Display all limit line segments for the maximum amplitude limit for noise data.

### Command syntax

```
CALCulate:LIMit:NOISe:MAXimum:DISPlay <boolean>
<boolean> :: = OFF | 0 | ON | 1
```

### Example

```
CALC:LIMit:NOISe:MAX:DISPlay ON
```

### Query syntax

```
CALC:LIMit:NOISe:MAX:DISPlay?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:NOISe:MAXimum:FAIL?

Query if the data type exceeds the limit type for the indicated segment.

### Command Syntax

Query Only

### Example

```
CALCulate:LIMit:NOISe:MAXimum:FAIL? 2
```

### Query syntax

```
CALCulate:LIMit:NOISe:MAXimum:FAIL? <segment_number>
<segment_number> ::= an integer in the range 1-100
```

### Return format

Boolean 0=Pass 1=Fail

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### Additional information

Returns 0 and an error message is generated if requested limit is not defined.  
Limit does not have to be displayed.

## **CALCulate:LIMit:NOISe:MAXimum:FAIL: ALL?**

Query if the data type exceeds the limit type for all defined segments.

### **Command Syntax**

Query Only

### **Example**

```
CALCulate:LIMit:NOISe:MAXimum:FAIL:ALL?
```

### **Query syntax**

```
CALCulate:LIMit:NOISe:MAXimum:FAIL:ALL?
```

### **Return format**

Boolean 0=Pass 1=Fail

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### **Additional information**

Limit does not have to be displayed to query.

## CALCulate:LIMit:NOISe:MINimum

Specifies a limit line segment for the minimum amplitude limit for noise data.

### Command syntax

```
CALCulate:LIMit:NOISe:MINimum <segment_number>, <start_offset>
[<frequency_suffix>], <start_power> [<power_suffix>], <stop_offset>
[<frequency_suffix>], <stop_power> [<power_suffix>]

<segment_number> ::= an integer in the range 1-100
<start_offset> ::= a real number (NRf data)
<start_power> ::= a real number (NRf data)
<stop_offset> ::= a real number (NRf data)
<stop_power> ::= a real number (NRf data)
```

### Example

```
CALC:LIMit:NOISe:MIN 1, 100, -50, 10e3, -80
```

### Query syntax

```
CALCulate:LIMit:NOISe:MINimum? <segment_number>
CALC:LIMit:NOISe:MIN? 1
```

### Return format

Real, Real, Real, Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: (all segments deleted)

SCPI Compliance: Instrument Specific.

### Additional information

Segment amplitude units are those of the current display graph type.

## CALCulate:LIMit:NOISe:MINimum:DELete

Delete the specified limit line segment for the minimum amplitude limit for noise data.

### Command syntax

```
CALCulate:LIMit:NOISe:MINimum:DELETE <segment_number>
<segment_number> ::= an integer in the range 1-100
```

### Example

```
CALC:LIMit:NOISe:MIN:DElete 1
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## **CALCulate:LIMit:NOISe:MINimum: DElete:ALL**

Delete all limit line segments for the minimum amplitude limit for noise data.

### **Command syntax**

`CALCulate:LIMit:NOISe:MINimum:DElete:ALL`

### **Example**

`CALC:LIMit:NOISe:MIN:DElete:ALL`

### **Query syntax**

Command Only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:NOISe:MINimum:DISPlay

Display all limit line segments for the minimum amplitude limit for noise data.

### Command syntax

```
CALCulate:LIMit:NOISe:MINimum:DISPlay <boolean>
<boolean> : := OFF | 0 | ON | 1
```

### Example

```
CALC:LIMit:NOISe:MIN:DISPlay ON
```

### Query syntax

```
CALC:LIMit:NOISe:MIN:DISPlay?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:NOISe:MINimum:FAIL?

Query if the data type exceeds the limit type for the indicated segment.

### Command Syntax

Query Only

### Example

```
CALCulate:LIMit:NOISe:MINimum:FAIL? 2
```

### Query syntax

```
CALCulate:LIMit:NOISe:MINimum:FAIL? <segment_number>
<segment_number> ::= an integer in the range 1-100
```

### Return format

Boolean 0=Pass 1=Fail

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### Additional information

Returns 0 and an error message is generated if requested limit is not defined.  
Limit does not have to be displayed.

## **CALCulate:LIMit:NOISe:MINimum: FAIL:ALL?**

Query if the data type exceeds the limit type for all defined segments.

### **Command Syntax**

Query Only

### **Example**

```
CALCulate:LIMit:NOISe:MINimum:FAIL:ALL?
```

### **Query syntax**

```
CALCulate:LIMit:NOISe:MINimum:FAIL:ALL?
```

### **Return format**

Boolean 0=Pass 1=Fail

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### **Additional information**

Limit does not have to be displayed to query.

## CALCulate:LIMit:SPUR:MAXimum

Specifies a limit line segment for the maximum amplitude limit for spur data.

### Command syntax

```
CALCulate:LIMit:SPUR:MAXimum <segment_number>, <start_offset>
[<frequency_suffix>], <start_power> [<power_suffix>], <stop_offset>
[<frequency_suffix>], <stop_power> [<power_suffix>]

<segment_number> ::= an integer in the range 1-100
<start_offset> ::= a real number (NRf data)
<start_power> ::= a real number (NRf data)
<stop_offset> ::= a real number (NRf data)
<stop_power> ::= a real number (NRf data)
```

### Example

```
CALC:LIMit:SPUR:MAX 1, 100, -50, 10e3, -80
```

### Query syntax

```
CALCulate:LIMit:SPUR:MAXimum? <segment_number>
CALC:LIMit:SPUR:MAX? 1
```

### Return format

Real, Real, Real, Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: (all segments deleted)

SCPI Compliance: Instrument Specific.

### Additional information

Segment amplitude units are those of the current display graph type.

## CALCulate:LIMit:SPUR:MAXimum:DELete

Delete the specified limit line segment for the maximum amplitude limit for spur data.

### Command syntax

```
CALCulate:LIMit:SPUR:MAXimum:DELete <segment_number>
<segment_number> ::= an integer in the range 1-100
```

### Example

```
CALC:LIMit:SPUR:MAX:DElete 1
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## **CALCulate:LIMIT:SPUR:MAXimum: DElete:ALL**

Delete all limit line segments for the maximum amplitude limit for spur data.

### **Command syntax**

`CALCulate:LIMIT:SPUR:MAXimum:DElete:ALL`

### **Example**

`CALC:LIMit:SPUR:MAX:DElete:ALL`

### **Query syntax**

Command Only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:SPUR:MAXimum:DISPlay

Display all limit line segments for the maximum amplitude limit for spur data.

### Command syntax

```
CALCulate:LIMit:SPUR:MAXimum:DISPlay <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
CALC:LIMit:SPUR:MAX:DISPLAY ON
```

### Query syntax

```
CALC:LIMit:SPUR:MAX:DISPLAY?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:SPUR:MAXimum:FAIL?

Query if the data type exceeds the limit type for the indicated segment.

### Command Syntax

Query Only

### Example

```
CALCulate:LIMit:SPUR:MAXimum:FAIL? 2
```

### Query syntax

```
CALCulate:LIMit:SPUR:MAXimum:FAIL? <segment_number>
<segment_number> ::= an integer in the range 1-100
```

### Return format

Boolean 0=Pass 1=Fail

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### Additional information

Returns 0 and an error message is generated if requested limit is not defined.  
Limit does not have to be displayed.

## CALCulate:LIMit:SPUR:MAXimum: FAIL:ALL?

Query if the data type exceeds the limit type for all defined segments.

### Command Syntax

Query Only

### Example

```
CALCulate:LIMit:SPUR:MAXimum:FAIL:ALL?
```

### Query syntax

```
CALCulate:LIMit:SPUR:MAXimum:FAIL:ALL?
```

### Return format

Boolean 0=Pass 1=Fail

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### Additional information

Limit does not have to be displayed to query.

## CALCulate:LIMit:SPUR:MINimum

Specifies a limit line segment for the minimum amplitude limit for noise data.

### Command syntax

```
CALCulate:LIMit:SPUR:MINimum <segment_number>, <start_offset>
[<frequency_suffix>], <start_power> [<power_suffix>], <stop_offset>
[<frequency_suffix>], <stop_power> [<power_suffix>]

<segment_number> ::= an integer in the range 1-100
<start_offset> ::= a real number (NRf data)
<start_power> ::= a real number (NRf data)
<stop_offset> ::= a real number (NRf data)
<stop_power> ::= a real number (NRf data)
```

### Example

```
CALC:LIMit:SPUR:MIN 1, 100, -50, 10e3, -80
```

### Query syntax

```
CALCulate:LIMit:SPUR:MINimum? <segment_number>
CALC:LIMit:SPUR:MIN? 1
```

### Return format

Real, Real, Real, Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: (all segments deleted)

SCPI Compliance: Instrument Specific.

### Additional information

Segment amplitude units are those of the current display graph type.

## CALCulate:LIMit:SPUR:MINimum:DELete

Delete the specified limit line segment for the minimum amplitude limit for spur data.

### Command syntax

```
CALCulate:LIMit:SPUR:MINimum:DELete <segment_number>
<segment_number> ::= an integer in the range 1-100
```

### Example

```
CALC:LIMit:SPUR:MIN:DElete 1
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## **CALCulate:LIMit:SPUR:MINimum: DElete:ALL**

Delete all limit line segments for the minimum amplitude limit for spur data.

### **Command syntax**

`CALCulate:LIMit:SPUR:MINimum:DElete:ALL`

### **Example**

`CALC:LIMit:SPUR:MIN:DElete:ALL`

### **Query syntax**

Command Only

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:NOISe:MINimum:DISPlay

Display all limit line segments for the minimum amplitude limit for spur data.

### Command syntax

```
CALCulate:LIMit:SPUR:MINimum:DISPlay <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
CALC:LIMit:SPUR:MIN:DISPlay ON
```

### Query syntax

```
CALC:LIMit:SPUR:MIN:DISPlay?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

## CALCulate:LIMit:SPUR:MINimum:FAIL?

Query if the data type exceeds the limit type for the indicated segment.

### Command Syntax

Query Only

### Example

```
CALCulate:LIMit:SPUR:MINimum:FAIL? 2
```

### Query syntax

CALCulate:LIMit:SPUR:MINimum:FAIL? <segment\_number>

<segment\_number> ::= an integer in the range 1-100

### Return format

Boolean 0=Pass 1=Fail

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### Additional information

Returns 0 and an error message is generated if requested limit is not defined.  
Limit does not have to be displayed.

## **CALCulate:LIMit:SPUR:MINimum: FAIL:ALL?**

Query if the data type exceeds the limit type for all defined segments.

### **Command Syntax**

Query Only

### **Example**

CALCulate:LIMit:SPUR:MINimum:FAIL:ALL?

### **Query syntax**

CALCulate:LIMit:SPUR:MINimum:FAIL:ALL?

### **Return format**

Boolean 0=Pass 1=Fail

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: N/A

SCPI Compliance: Instrument Specific.

### **Additional information**

Limit does not have to be displayed to query.

## CALCulate:PBWidth

Power Bandwidth adjustment.

### Command syntax

```
CALCulate:PBWidth <number>
<number> ::= a real number (NRf data)
```

### Query syntax

```
CALCulate:PBWidth?
```

### Example

```
CALCulate:PBWidth 100
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1 Hz

SCPI Compliance: Instrument Specific.

### Additional information

Applied to data output by CALCulate:DATA? when outputting:

CALCulate:VIEW:TRACe (start, stop, #points, distribution(log/linear)) or  
CALCulate:VIEW:XYData

## CALCulate:SElect

Specify which data set is selected for return by:

- CALCulate:DATA?
- CALCulate:ACCumulated[:PHASe]? (tau, start-offset, stop-offset)
- CALCulate:AVARiance? (tau, Frequency offset)
- CALCulate:TVARIANCE? (tau, Frequency offset)

### Command syntax

```
CALCulate:SElect BOTH|NOISE|SPURS
```

### Example

```
CALCulate:SElect NOISE
```

### Query syntax

```
CALCulate:SElect?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: BOTH

SCPI Compliance: Instrument Specific.

### Additional information

- BOTH = return both noise and spur data
- NOISE = return noise data only
- SPURS = return spur data only

## **CALCulate:SMOothing**

Specify the degree of smoothing to be applied to data.

### **Command syntax**

```
CALCulate:SMOothing <number>
<number> ::= an integer (NRF data)
```

### **Example**

```
CALCulate:SMOothing 2
```

### **Query syntax**

```
CALCulate:SMOothing?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Instrument Specific.

### **Additional information**

Smoothing performs a running average on each data point. The smoothing value is the number of points to average on each side of the current data point. Thus, the number of points averaged is:

$2*n+1$  where n is the value used for smoothing

Applied to data output by CALCulate:DATA? when outputting:

CALCulate:VIEW:TRACe (start, stop, #points, distribution(log/linear)) or  
CALCulate:VIEW:XYData

## CALCulate:TRANSform

Specify the graph type transform for CALCulate:DATA?

### Command syntax

```
CALCulate:TRANSform SSBNoise|SDPF|SDFF|SFFF|NF2Port|AMNoise|BBAND
```

SSBNoise	= Single Sideband Noise (dBc/Hz)
SDPF	= Spectral Density of Phase Fluctuations (dB/Hz)
SDFF	= Spectral Density of Frequency Fluctuations (Hz/Sqrt(Hz))
SFFF	= Spectral Density of Fractional Frequency Fluctuations (1/Sqrt(Hz))
NF2Port	= Noise Figure for a 2-Port device (dB)
AMNoise	= AM Noise (dB)
BBAND	= Base Band Noise (dB)

### Example

```
CALCulate:TRANSform BBAND
```

### Query syntax

```
CALCulate:TRANSform?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: SSBNoise

SCPI Compliance: Instrument Specific.

## CALCulate:TVARiance?

Jitter.

### Command Syntax

Query Only

#### Query syntax

```
CALCulate:TVARiance? <tau>,<upper_offset>
<tau> ::= a real number (NRf data)
<upper_offset> ::= a real number (NRf data)
```

#### Return format

Real

#### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

#### Additional information

Performs calculation on currently selected data as specified by:

CALCulate:SElect (BOTH | NOISe | SPURs)

## CALCulate:VIEW:SPURtable

Specifies the list of spurs returned by CALCulate:DATA?. The list of spurs is returned as a list of frequency/amplitude pairs.

### Command syntax

```
CALCulate:VIEW:SPURtable
```

### Example

```
CALCulate:VIEW:SPURtable
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

### Additional information

When this view is specified, results returned by CALCulate:DATA? are affected by the following:

- CALCulate:TRANSform
- CALCulate:YShift

## **CALCulate:VIEW:TRACe**

Specifies that trace data be returned by CALCulate:DATA?.

### **Command syntax**

```
CALCulate:VIEW:TRACe <start_offset> [<frequency_suffix>],  
                      <stop_offset> [<frequency_suffix>],  
                      <points>,  
                      <distribution>  
  
<start_offset> ::= a real number (NRf data)  
<stop_offset> ::= a real number (NRf data)  
<frequency_suffix> ::= Hz|kHz|MHz|GHz  
<points> ::= an integer (NRf data)  
<distribution> ::= LOG|LINEar
```

### **Example**

```
CALCulate:VIEW:TRACe 10Hz, 100kHz, 1000, LOG
```

### **Query syntax**

```
CALCulate:VIEW:TRACe
```

### **Return format**

Frequency/amplitude pairs.

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

### **Additional information**

CALCulate:VIEW:TRACe data is interpolated between start and stop offsets to provide data for the requested distribution (log or linear) and number of points. If you want the actual measured data points use CALCulate:VIEW:XYData.

## CALCulate:VIEW:XYData

Specifies that data triples be returned by CALCulate:DATA? for the user-defined measurement range.

### Command syntax

```
CALCulate:VIEW:XYData
```

### Example

```
CALCulate:VIEW:XYData
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

### Additional information

Returns measured data points.

## CALCulate:YShift

The specified amplitude adjustment is applied to data returned by CALCulate:DATA?.

### Command syntax

```
CALCulate:YShift <number> [dB]  
<number> ::= a real number (NRf data)
```

### Example

```
CALCulate:YShift 2
```

### Query syntax

```
CALCulate:YShift?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0.0

SCPI Compliance: Instrument Specific.

### Additional information

Applied to data output by CALCulate:DATA? when outputting:

- CALCulate:VIEW:SPURtable
- CALCulate:VIEW:TRACe (start, stop, #points, distribution (log/linear)) or
- CALCulate:VIEW:XYData

## 8

# CALibrate Commands

- CALlibrate Commands Introduction [146](#)
- CALlibrate:DETector:CONSTant [147](#)
- CALlibrate:DETector:CONSTant:METHod [148](#)
- CALlibrate:DETector:CONSTant:SPUR:AMPLitude [150](#)
- CALlibrate:DETector:CONSTant:SPUR:OFFSet [151](#)
- CALlibrate:VCO:IRESistance [152](#)
- CALlibrate:VCO:PLLSuppress [153](#)
- CALlibrate:VCO:PLLSuppress:APOLe? [155](#)
- CALlibrate:VCO:PLLSuppress:CBWidth? [156](#)
- CALlibrate:VCO:PLLSuppress:DISPlay [:ALWays] [157](#)
- CALlibrate:VCO:PLLSuppress:ERRor [158](#)
- CALlibrate:VCO:PLLSuppress:ERRor:ACTion [159](#)
- CALlibrate:VCO:PLLSuppress:PTRange? [160](#)
- CALlibrate:VCO:TCONSTant? [161](#)
- CALlibrate:VCO:TCONSTant:METHod [162](#)
- CALlibrate:VCO:TCONSTant:NOMinal [164](#)
- CALlibrate:VCO:TMODE [165](#)
- CALlibrate:VCO:VCADjust [166](#)
- CALlibrate:VCO:VCENTER [167](#)
- CALlibrate:VCO:VRANGE [168](#)



## CALlibrate Commands Introduction

The calibration process for a phase lock loop measurement involves determining the phase Detector Constant, the VCO Tune Constant, and verifying the Loop Suppression. The phase Detector Constant is the sensitivity of the phase detector expressed in volts per radian (V/Rad). The VCO Tune Constant is the sensitivity of the tuning input of the Voltage Controlled Oscillator (VCO) expressed in Hertz per volt (Hz/V). The Loop Suppression verification characterizes the phase lock loop configured for the measurement and then compares the measured loop response with a theoretical loop suppression curve.

The commands in this subsystem have the following command hierarchy:

- CALibrate:DETector:CONSTant (value)
- CALibrate:DETector:CONSTant:METHod (BEATnote | DCPeak | SSPur | DSPur | FMD | AMIN | PSHift | NONE)
- CALibrate:DETector:CONSTant:SPUR:AMPLitude (value)
- CALibrate:DETector:CONSTant:SPUR:OFFSet (value)
- CALibrate:VCO:IRESistance (value)
- CALibrate:VCO:PLLSuppress?
- CALibrate:VCO:PLLSuppress:APOLe?
- CALibrate:VCO:PLLSuppress:CBWidth?
- CALibrate:VCO:PLLSuppress (0 | OFF | 1 | ON)
- CALibrate:VCO:PLLSuppress:DISPLAY[:ALways] (0 | OFF | 1 | ON)
- CALibrate:VCO:PLLSuppress:ERRor (value)
- CALibrate:VCO:PLLSuppress:ERRor:ACTion (THEoretical | ADJusted | PAUSe)
- CALibrate:VCO:PLLSuppress:PTRange?
- CALibrate:VCO:TCONstant?
- CALibrate:VCO:TCONstant:METHod (CURRent | MEASure | CALCulate)
- CALibrate:VCO:TCONstant:NOMinal (value)
- CALibrate:VCO:TMODE (EFC | DCFM)
- CALibrate:VCO:VCADjust (value)
- CALibrate:VCO:VCENter (value)
- CALibrate:VCO:VRANge (value)

## CALibrate:DETector:CONSTant

Specify the detector constant in Volts / Radian.

### Command syntax

```
CALibrate:DETector:CONSTant <number>
<number> ::= a real number (NRF data)
```

### Example

```
CALibrate:DETector:CONSTant 1.5E-6
```

### Query syntax

```
CALibrate:DETector:CONSTant?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1E-6

SCPI Compliance:Instrument Specific.

### Additional information

The phase detector translates relative phase fluctuations between the two phase detector inputs to voltage fluctuations. The amplitude of the phase detector's output voltage is proportional to the amount of relative phase fluctuation at its two inputs scaled by and the sensitivity of the detector. The phase detector's sensitivity is the phase Detector Constant. The phase Detector Constant determines the absolute noise floor of the test system. The accuracy of the Phase Lock Loop measurement is dependent on the accuracy of the phase Detector Constant.

Use the Current Detector Constant and Measure the Detector Constant are the two methods available for determining the phase Detector Constant.

## CALibrate:DETector:CONStant:METHod

This command is used to specify the method by which to measure the detector constant.

### Command syntax

```
CALibrate:DETector:CONStant:METHod BEATnote|DCPeak|SSPur  
|DSPur|FMDeviation|AMINternal|PSHift|NONE
```

### Example

```
CALibrate:DETector:CONStant:METHod FM Deviation
```

### Query syntax

```
CALibrate:DETector:CONStant:METHod?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: BEATnote

SCPI Compliance: Instrument Specific.

### Additional information

- BEATnoteDerive from measured beatnote
- DCPeakDerive from measured +/- DC peak voltage
- SSPurDerive from single-sided spur
- DSPurDerive from double-sided spur
- FMDeviation Derive from FM rate and deviation
- AMINternal Use AM internal automatic self-calibration.
- NONEUse the current detector constant

A subset of the detector constant methods is valid for each measurement type as follows:

- ABSolute(Phase Noise using a Phase Locked Loop)
  - NONEUse the current detector constant
  - BEATnoteDerive from measured beatnote
- RESidual(Phase Noise without using a Phase Locked Loop)
  - NONEUse the current detector constant
  - BEATnoteDerive from measured beatnote
  - DCPeakDerive from measured +/- DC peak voltage
  - SSPurDerive from single-sided spur
  - DSPurDerive from double-sided spur
- FMDiscriminator (Phase Noise using an FM Discriminator)
  - NONEUse the current detector constant
  - DSPurDerive from double-sided spur
  - FMDeviationDerive from FM rate and deviation
- AM (AM Noise Measurement)
  - NONEUse the current detector constant
  - AMInternal Use AM internal automatic self-calibration.
  - SSPurDerive from single-sided spur
  - DSPurDerive from double-sided spur
- BBANDBase Band Noise Measurement
  - The detector constant method is not applicable for baseband noise measurements.
- NOTSet (Base Band Noise Measurement without using the Test Set)
  - The detector constant method is not applicable for baseband noise measurements.

## **CALibrate:DETector:CONSTant:SPUR: AMPLitude**

Specify the spur amplitude used to measure the detector constant when the detector constant method is set to SSPUR or DSPUR.

### **Command syntax**

```
CALibrate:DETector:CONSTant:SPUR:AMPLitude <number> [dB]  
<number> ::= a real number (NRf data)
```

### **Example**

```
CALibrate:DETector:CONSTant:SPUR:AMPLitude -100
```

### **Query syntax**

```
CALibrate:DETector:CONSTant:SPUR:AMPLitude?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: -130

SCPI Compliance:Instrument Specific.

## CALibrate:DETector:CONSTant:SPUR:OFFSet

Specify the spur offset frequency used to measure the detector constant when the detector constant method is set to SSPUR or DSPUR.

### Command syntax

```
CALibrate:DETector:CONSTant:SPUR:OFFSet <number> [Hz|kHz|MHz|GHz]  
<number>      ::= a real number (NRF data)
```

### Example

```
CALibrate:DETector:CONSTant:SPUR:OFFSet 10
```

### Query syntax

```
CALibrate:DETector:CONSTant:SPUR:OFFSet?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1 Hz

SCPI Compliance:Instrument Specific.

## **CALibrate:VCO:IRESistance**

Specify the input resistance of the VCO.

### **Command syntax**

```
CALibrate:VCO:IRESistance <number> [OHMS | KOHMS | MOHMS]  
<number> ::= a real number (NRF data)
```

### **Example**

```
CALibrate:VCO:IRESistance 500E3
```

### **Query syntax**

```
CALibrate:VCO:IRESistance?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 1E6 Ohms

SCPI Compliance: Instrument Specific.

### **Additional information**

VCO Tune Port Input Resistance is the input impedance of the VCO's tune port. This entry must be accurate to within +/-5% when the VCO Tune Constant is not going to be measured. When the Tune Constant is going to be measured by the software, the actual value of the VCO Tune Port Input Resistance is not critical, and an entry of 1E+6 is recommended.

## CALibrate:VCO:PLLSuppress

Enable/disable PLL suppression verification.

Phase Lock Loop Suppression verification can be turned on or off. Verification of the Phase Lock Loop Suppression insures that the Phase Lock Loop Bandwidth (PLL BW), the Phase Detector Constant, and the VCO Tune Constant are all accurate for the measurement. (Note that the software always corrects for the loop suppression whether or not verification is selected.)

### Command syntax

```
CALibrate:VCO:PLLSuppression <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
CALibrate:VCO:PLLSuppression OFF
```

### Query syntax

```
CALibrate:VCO:PLLSuppression?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ON

SCPI Compliance:Instrument Specific.

### Additional information

Verification of the Phase Lock Loop Suppression insures that the Phase Lock Loop Bandwidth (PLL BW), the Phase Detector Constant, and the VCO Tune Constant are all accurate for the measurement. (Note that the software always corrects for the loop suppression whether or not verification is selected.)

The software verifies Loop Suppression before beginning the measurement by closing the phase lock loop and injecting noise into the loop. The response of the loop is measured and recorded. The loop is then opened, and a measurement is made of the open loop response. The suppression of the PLL is the difference between the closed loop response and open loop response to the injected noise. The measured Loop Suppression curve is smoothed and then

four points are selected along the curve including the peak and the 8 dB point. The measured curve is then compared to the theoretical curve at the four selected points.

The amount of adjustment required to fit the theoretical curve to the measured curve is recorded as the PLL GAIN CHANGE on the Suppression Graph and the frequency of the Assumed Pole. The Assumed Pole is a software controlled term used to fit the Adjusted Theoretical loop response to the smoothed measured response of the phase lock loop. The MAX ERROR is the final amount of error existing between the adjusted theoretical curve and the measured curve of the phase lock loop suppression. If the PLL GAIN CHANGE or MAX ERROR is greater than 1 dB, the test system indicates that an Accuracy Specification Degradation has been detected.

Verification of the loop suppression may be prevented by excessive noise close to the carrier, by a large spur within the bandwidth of the PLL, or by injection locking.

It should be assumed that an indicated Accuracy Specification Degradation applies at all offset frequencies (both inside and outside of the loop bandwidth).

If the Detector Constant and VCO Tune Constant are known to be accurate, the PTR is less than 10 MHz, and the VCO tuning port bandwidth is greater than PLL BW X 10, then a measurement without Loop Suppression Verification will be accurate.

## CALibrate:VCO:PLLSuppress:APOLe?

This is the frequency of the Assumed Pole required to adjust the theoretical loop suppression to match the smoothed measured Loop Suppression. The Assumed Pole frequency is normally much greater than the PLL BW.

### Query syntax

```
CALibrate:VCO:PLLSuppress:APOLe?
```

### Return format

Real (Hz)

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: n/a

SCPI Compliance: Instrument Specific.

### Additional information

If the Assumed Pole is adjusted to a frequency of less than 10 X PLL BW, peaking in the PLL suppression is indicated. For PLL BWs less than 20 kHz, an Assumed Pole of less than 10 X PLL BW indicates a delay or phase shift in the VCO Tune Port. For PLL BWs greater than 20 kHz, the Assumed Pole may be adjusted to less than 10 X PLL BW to account for phase shifts in the test set.

Also see: CALibrate:VCO:PLLSuppress

## CALibrate:VCO:PLLSuppress:CBWidth?

This is the predicted Phase Lock Loop Bandwidth for the measurement. The predicted PLL BW is based on the predicted PTR. The Closed PLL BW will not be adjusted as a result of an accuracy degradation. If an accuracy degradation is detected, the amount of error is determined from either the PLL Gain Change or the Maximum Error, which ever is larger. The degradation itself is 1 dB less than the greater of these.

### Query syntax

```
CALibrate:VCO:PLLSuppress:CBWidth?
```

### Return format

Real (Hz)

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: n/a

SCPI Compliance: Instrument Specific.

### Additional information

Also see: CALibrate:VCO:PLLSuppress

## CALibrate:VCO:PLLSuppress:DISPlay[:ALWays]

When turned ON, the PLL suppression graph will be displayed each time PLL suppression verification is performed. When turned OFF, the PLL suppression graph is displayed only when the suppression error is out of bounds.

### Command syntax

```
CALibrate:VCO:PLLSuppress:DISPlay[:ALWays] <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
CALibrate:VCO:PLLSuppress:DISPlay ON
```

### Query syntax

```
CALibrate:VCO:PLLSuppress:DISPlay?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

## **CALibrate:VCO:PLLSuppress:ERRor**

Specify the acceptable error for PLL suppression verification.

The Maximum Suppression Error Limit is the final amount of error existing between the adjusted theoretical curve and the measured curve of the phase lock loop suppression.

### **Command syntax**

```
CALibrate:VCO:PLLSuppress:ERRor <number> [dB]
```

### **Example**

```
CALibrate:VCO:PLLSuppress:ERRor .5
```

### **Query syntax**

```
CALibrate:VCO:PLLSuppress:ERRor?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 1 dB

SCPI Compliance: Instrument Specific.

## CALibrate:VCO:PLLSuppress:ERRor:ACTion

Specify which PLL suppression curve to use in the case that PLL suppression verification fails.

### Command syntax

```
CALibrate:VCO:PLLSuppress:ERRor:ACTion THEoretical|ADJusted|PAUSE
```

### Example

```
CALibrate:VCO:PLLSuppress:ERRor:ACTion THEoretical
```

### Query syntax

```
CALibrate:VCO:PLLSuppress:ERRor:ACTion?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: THEoretical

SCPI Compliance: Instrument Specific.

### Additional information

See CALibrate:VCO:PLLSuppress:ERRor.

## CALibrate:VCO:PLLSuppress:PTRange?

This is the Peak Tuning Range (PTR) for the measurement determined from the VCO Tune Constant and the Tune Range of VCO. This is the key parameter in determining the PLL properties, the Drift tracking Range, and the ability to phase lock sources with high close in noise.

### Query syntax

```
CALibrate:VCO:PLLSuppress:PTRange?
```

### Return format

Real (Hz)

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: n/a

SCPI Compliance: Instrument Specific.

### Additional information

The PTR value displayed should be approximately equal to the product of the VCO Tune Constant times the Tune Range of VCO. This will not be the case when a significant Accuracy Specification Degradation is detected (> 4 db) by the Loop Suppression Verification. For Accuracy Specification Degradations of >4 db, the PTR and Assumed Pole are adjusted when the theoretical loop suppression is fit to the smoothed measured Loop Suppression. In these cases, the test system displays the adjusted PTR.

Any time the PTR must be adjusted by more than 1 db (as indicated by an Accuracy Specification Degradation of greater than 0 db) it is an indication that the phase Detector Constant or the VCO Tune Constant will be in error at frequency offsets near the PLL BW, or that the PLL BW is being affected by some other problem such as injection locking.

Also see: CALibrate:VCO:PLLSuppress

## CALibrate:VCO:TCONstant?

Query the VCO tune constant (which was determined by the calibration method).

### Command Syntax

Query Only

#### Query syntax

```
CALibrate:VCO:TCONstant?
```

#### Return format

Real (Hz/Volt)

#### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1E6

SCPI Compliance: Instrument Specific.

#### Additional information

The VCO Tune Constant is the frequency sensitivity of the VCO source to voltage changes at its control voltage input. This constant is measured in Hz/V. The software uses the VCO Tune Constant along with the defined Tune Range of VCO and the VCO's Tune Port Input Resistance to determine the Peak Tuning Range for the measurement. The Bandwidth of the Phase Lock Loop, the Lock Capture Range, and the Drift Tracking Range for the measurement are all derived from the Peak Tuning Range. Three calibration techniques are available for determining the VCO Tune Constant for the measurement; Use current VCO tuning sensitivity, Measure the VCO tuning sensitivity, Calculate from the expected VCO tuning sensitivity using the Tune Port Resistance.

## CALibrate:VCO:TCONstant:METHod

Specify the method used to determine the VCO tune constant.

### Command syntax

```
CALibrate:VCO:TCONstant:METHod CURRent|MEASure|CALCulate
```

### Example

```
CALibrate:VCO:TCONstant:METHod?
```

### Query syntax

```
CALibrate:VCO:TCONstant:METHod MEASure
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: MEASure

SCPI Compliance: Instrument Specific.

### Additional information

#### CURRent

This calibration method uses the value of the VCO Tune Constant currently in memory. Selecting this method saves time for measuring the VCO Tune Constant without any degradation in accuracy, providing either the same VCO source is being used or a source with an identical tuning constant is being used (within +/- 5%).

#### MEASure

Selecting this calibration method causes the test system to automatically measure the tuning sensitivity and tuning linearity of the VCO source. Measuring the VCO Tune Constant is the recommended method under most circumstances for ensuring measurement accuracy. The test system cannot measure the VCO Tune Constant for an entered Peak Tuning Range greater than 500 kHz for test systems configured without an RF Analyzer, and 200 MHz for test systems configured with an RF Analyzer.

When measuring the VCO Tune Constant, the test system requires that the VCO Tune Constant defined in the Measurement Definition, Sources tab window be within a factor of two of the VCO's actual sensitivity. This approximation is required in order for the software to establish a beatnote. The frequency response of the VCO source must remain flat (+/- 3 dB) from DC to the phase lock loop bandwidth (PLL BW).

### CALCulate

Selecting the Calculate from Expected Tune Constant method causes the test system to use the entered VCO Tune Constant and VCO Tune Port Input Resistance that have been entered in the Measurement Definition, Sources tab window. This method requires that the entered VCO Tune Constant is within +/- 5% of the VCO's actual sensitivity. If it is not, the test system reports an Accuracy Specification Degradation after verifying the Phase Lock Loop Suppression.

$$\text{VCO Tuning Constant} = \text{Expected Tuning Constant} * (\text{Rin} / (\text{Rin} + 50))$$

Where: Rin = VCO Tune Port Input Resistance

## CALibrate:VCO:TCONstant:NOMinal

Specify the nominal value used to calculate the VCO tune constant.

### Command syntax

```
CALibrate:VCO:TCONstant:NOMinal <number>
<number> ::= a real number (NRF data)
```

### Example

```
CALibrate:VCO:TCONstant:NOMinal 2e3
```

### Query syntax

```
CALibrate:VCO:TCONstant:NOMinal?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 10E3

SCPI Compliance: Instrument Specific.

### Additional information

VCO Tune Constant is the resulting frequency deviation of the Voltage Controlled Oscillator (VCO) for a 1 volt change at its tune port. This entry must be accurate to within +/-5% when the phase noise software is not going to measure the VCO Tune Constant. The entry must be accurate to within a factor of 2 when the VCO Tune Constant is going to be measured by the software.

## CALibrate:VCO:TMode

Specify the VCO tune mode. The VCO is the source to which the tune voltage is applied as specified in [SENSe:]TVCO REference|CARRier.

### Command syntax

```
CALibrate:VCO:TMode EFC|DCFM
```

### Example

```
CALibrate:VCO:TMode EFC
```

### Query syntax

```
CALibrate:VCO:TMode?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: EFC

SCPI Compliance: Instrument Specific.

### Additional information

- EFC - Electronic Frequency Control
- DCFM - DC Frequency Modulation

#### NOTE

Not all VCO's support tuning by means of DC FM.

## **CALibrate:VCO:VCADjust**

Specify the allowable adjustment range (from the VCO's center voltage).

### **Command syntax**

```
CALibrate:VCO:VCADjust <number> [V]  
<number> ::= a real number (NRf data)
```

### **Example**

```
CALibrate:VCO:VCADjust 2.5
```

### **Query syntax**

```
CALibrate:VCO:VCADjust?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 1 V

SCPI Compliance: Instrument Specific.

## CALibrate:VCO:VCENter

Specifies the center voltage for the VCO.

### Command syntax

```
CALibrate:VCO:VCENter <number> [V]
<number> ::= a real number (NRF data)
```

### Example

```
CALibrate:VCO:VCENter 1.5
```

### Query syntax

```
CALibrate:VCO:VCENter?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0 Volts

SCPI Compliance:Instrument Specific.

### Additional information

Center Voltage of VCO Tune Curve is the center voltage of the tuning curve of the VCO, that is, the voltage required at the tune port input to set the VCO to the desired carrier frequency for the measurement. A 0 volt entry allows the maximum Voltage Tune Range available from the test set. Entries other than zero restrict the Voltage Tune Range as described below:

**Table 2** Voltage Tune Range

Center Voltage	Maximum Voltage Tuning Range
<= 2V	+/-10V
> 2V	+/-12V - Center Voltage

## CALibrate:VCO:VRANge

Specifies the tuning voltage range for the VCO.

### Command syntax

```
CALibrate:VCO:VRANge <number> [V]
<number> ::= a real number (NRF data)
```

### Example

```
CALibrate:VCO:VRANge 4.5
```

### Query syntax

```
CALibrate:VCO:VRANge?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1 Volts

SCPI Compliance: Instrument Specific.

### Additional information

This is the defined Tune Range of VCO through which the test system may tune the VCO around the Center Voltage. The VCO output must not change in amplitude by greater than 1 dB, show any reversal in frequency tuning, or be susceptible to damage within the defined Tune Range around the Center Voltage.

For the phase noise software to measure the VCO Tune Constant accurately, the VCO must tune monotonically across +/-45% of the Tune Range of VCO around the Center Voltage, and the slope must not go to zero. If the VCO Tune Constant is not measured by the test system, the VCO must tune to within +/-10% of the Tune Range of VCO around the Center Voltage using the defined VCO Tune Constant.

To protect the VCO from possible damage, the Tune Voltage output port should not be connected to the VCO's input port until the Connect diagram is displayed.

VCO Tuning Constant \* Voltage Tuning Range = Peak Tuning Range

9

## DISPlay Commands

- [DISPlay Commands Introduction 170](#)
- [DISPlay:GRAPh:BOUNds:AMPLitude 171](#)
- [DISPlay:GRAPh:BOUNds:AMPLitude? 173](#)
- [DISPlay:GRAPh:BOUNds:FREQuency 174](#)
- [DISPlay:GRAPh:CFSCale 175](#)
- [DISPlay:GRAPh:DIPower 176](#)
- [DISPlay:GRAPh:PBWidth 177](#)
- [DISPlay:GRAPh:SMOothing 178](#)
- [DISPlay:GRAPh:TRANSform 179](#)
- [DISPlay:GRAPh:YShift 180](#)
- [DISPlay:MEASurement:TIME? 181](#)
- [DISPlay:TEXT:TITLe 182](#)



## DISPlay Commands Introduction

Use the DISPLAY commands to control the display of data in the Measurement Development Client GUI. These commands only effect the display presented to the user and do NOT effect data output by CALCulate:DATA? or DATA? queries. Similar commands are available in the CALCulate tree.

Selection and presentation of textual, graphical, and TRACe information. This information includes measurement data, user-interaction display, and data presented to the instrument by the controller. DISPLAY is independent of, and does not modify, how data is returned to the controller.

The commands in this subsystem have the following command hierarchy:

- DISPlay:GRAPh:BOUNds:AMPLitude? (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
  - DISPlay:GRAPh:BOUNds:AMPLitude (Transform,Min,Max)
  - DISPlay:GRAPh:BOUNds:FREQuency (Min,Max)
  - DISPlay:GRAPh:CFSCale (value)
  - DISPlay:GRAPh:DIPower (value)
  - DISPlay:GRAPh:PBWidth (value)
  - DISPlay:GRAPh:SMOothing (value)
  - DISPlay:GRAPh:TRANSform (SSBN | SDPF | SDFF | SFFF | NF2P | AMN | BBAN)
  - DISPlay:GRAPh:YSHift (value)
  - DISPlay:MEASurement:TIME?
  - DISPlay:TEXT:TITLe ("string")

## DISPlay:GRAPh:BOUNds:AMPLitude

Amplitude coordinate units and bounds of graphical display.

### Command syntax

```
DISPlay:GRAPh:BOUNds:AMPLitude <transform>,<Ymin>,<Ymax>
<transform> ::= SSBNoise|SDPF|SDFF|SFFF|NF2Port|AMNoise|BBAND
    • SSBNoise = Single Sideband Noise (dBc/Hz)
    • SDPF = Spectral Density of Phase Fluctuations (dB/Hz)
    • SDFF = Spectral Density of Frequency Fluctuations (Hz/Sqrt(Hz))
    • SFFF = Spectral Density of Fractional Frequency Fluctuations
              (Hz/Sqrt(Hz))
    • NF2Port = Noise Figure for a 2-Port device (dB)
    • AMNoise = AM Noise (dB)
    • BBAND = Base Band Noise (dB)
<Ymin> ::= a real number (NRf data)
           limits:
<Ymax> ::= a real number (NRf data)
           limits:
```

### Command Example

```
DISPlay:GRAPh:BOUNds:AMPLitude -150,0
```

### Query syntax

```
DISPlay:GRAPh:BOUNds:AMPLitude? <transform>
<transform> ::= SSBNoise|SDPF|SDFF|SFFF|NF2Port|AMNoise|BBAND
```

### Query Example

```
DISPlay:GRAPh:BOUNds:AMPLitude? SDFF
```

### Return format

Real, Real

## **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: SSBNoise, -170, 0

SCPI Compliance: Instrument Specific.

## DISPlay:GRAPh:BOUNds:AMPLitude?

Amplitude coordinate units and bounds of graphical display.

### Command Syntax

Query Only

### Query syntax

```
DISPlay:GRAPh:BOUNds:AMPLitude? <transform>,<Ymin>,<Ymax>
<transform> ::= SSBNoise|SDPF|SDFF|SFFF|NF2Port|AMNoise|BBAND
```

### Example

```
DISPlay:GRAPh:BOUNds:AMPLitude SDFF
```

### Return format

Real, Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: SSBNoise, -170, 0

SCPI Compliance: Instrument Specific.

## **DISPlay:GRAPh:BOUNds:FREQuency**

Frequency coordinate bounds of graphical display.

### **Command syntax**

```
DISPlay:GRAPh:BOUNds:FREQuency <Xmin>,<Xmax>
<Xmin> ::= a real number (NRf data)
<Xmax> ::= a real number (NRf data)
```

### **Example**

```
DISPlay:GRAPh:BOUNds:FREQuency 10, 100E3
```

### **Query syntax**

```
DISPlay:GRAPh:BOUNds:FREQuency?
```

### **Return format**

Real, Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 1, 10E6

SCPI Compliance: Instrument Specific.

## **DISPlay:GRAPH:CFSCale**

Specify the Carrier Frequency SCale multiplier used for displaying the graph.

### **Command syntax**

```
DISPlay:GRAPH:CFSCale <number>
<number> ::= a real number (NRf data)
```

### **Example**

```
DISPlay:GRAPH:CFSCale 2.0
DISPlay:GRAPH:CFSCale 0.5
```

### **Query syntax**

```
DISPlay:GRAPH:CFSCale?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 1.0

SCPI Compliance: Instrument Specific.

### **Additional information**

The carrier frequency scaling function allows you to plot results based on frequency changes in the carrier, and to plot the noise of the measured source to a translated frequency. The scale factor can be any number greater than zero. Entering a factor-of-2 doubles the frequency, a factor-of-3 triples the frequency, and so on. A number less than one corresponds to a scaling to a lower carrier frequency.

Plots made after the scale factor has been entered indicate noise for the scaled frequency. Noise levels increase for scale factors > 1 and decrease for factors <1.

## **DISPlay:GRAPh:DIPower**

Specify the power present at the input of the DUT in dBm.

### **Command syntax**

```
DISPlay:GRAPh:DIPower <number>
<number> ::= a real number (NRf data)
```

### **Example**

```
DISPlay:GRAPh:DIPower -10
```

### **Query syntax**

```
DISPlay:GRAPh:DIPower?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Instrument Specific.

## DISPlay:GRAPh:PBWidth

Specify the trace power bandwidth adjustment used in displaying the graph.

### Command syntax

```
DISPlay:GRAPh:PBWidth <number>
<number> ::= a real number (NRf data)
```

### Example

```
DISPlay:GRAPh:PBWidth 100 Hz
```

### Query syntax

```
DISPlay:GRAPh:PBWidth?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1.0 Hz

SCPI Compliance: Instrument Specific.

### Additional information

This function specifies the bandwidth frequency the trace data will be normalized to. Because phase noise is usually specified in a 1 Hz bandwidth, the measurement result must also be corrected for the equivalent noise bandwidth for the analyzer. This bandwidth normalization process requires subtracting  $10 \log$  (equivalent noise in Hz) from the measured value. For example, if a value of -123 dBc is obtained from a measurement with an analyzer equivalent noise bandwidth of 1.2 kHz, this value must be corrected by subtracting  $10 \log (1200)$ , yielding -153.8 dBc/Hz.

## **DISPlay:GRAPh:SMOothing**

Specify the degree of smoothing used in displaying the graph.

### **Command syntax**

```
DISPlay:GRAPh:SMOothing <number>
<number> ::= an integer (NRF data)
```

### **Example**

```
DISPlay:GRAPh:SMOothing 5
```

### **Query syntax**

```
DISPlay:GRAPh:SMOothing?
```

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Instrument Specific.

### **Additional information**

Smoothing performs a running average on each data point. The smoothing value is the number of points to average on each side of the displayed data point. Thus, the number of points averaged is:

$2*n+1$  where n is the value used for smoothing

## DISPlay:GRAPH:TRANsform

Specify the transformation used to display data on the graph.

### Command syntax

```
DISPlay:GRAPH:TRANSform SSBNoise|SDPF|SDFF|SFFF|NF2Port|AMNoise|BBAND
```

### Example

```
DISPlay:GRAPH:TRANSform SFFF
```

### Query syntax

```
DISPlay:GRAPH:TRANSform?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: SSBNoise

SCPI Compliance: Instrument Specific.

### Additional information

- SSBNoise = Single Sideband Noise (dBc/Hz)
- SDPF = Spectral Density of Phase Fluctuations (dB/Hz)
- SDFF = Spectral Density of Frequency Fluctuations (Hz/Sqrt(Hz))
- SFFF = Spectral Density of Fractional Frequency Fluctuations 1/Sqrt(Hz))
- NF2Port = Noise Figure for a 2-Port device (dB)
- AMNoise = AM Noise (dB)
- BBAND = Base Band Noise (dB)

## **DISPlay:GRAPh:YSHift**

Specify the amplitude offset used in displaying the graph.

### **Command syntax**

```
DISPlay:GRAPh:YSHift <number> [dBc]  
<number> ::= a real number (NRf data)
```

### **Example**

```
DISPlay:GRAPh:YSHift 2.0
```

### **Query syntax**

```
DISPlay:GRAPh:YSHift?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State:0.0 dBm

SCPI Compliance: Instrument Specific.

## DISPlay:MEASurement:TIME?

The date, start time and stop time of the current measurement.

### Query syntax

```
DISPlay:MEASurement:TIME?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: n/a

SCPI Compliance: Instrument Specific.

### Additional information

Example: 29 Jul 1997 16:51:57 - 16:53:19

## **DISPlay:TEXT:TITLe**

Title of the measurement.

### **Command syntax**

DISPlay:TEXT:TITLe <“string”>

### **Query syntax**

DISPlay:TEXT:TITLe?

### **Example**

DISPlay:TEXT:TITLe “Absolute Phase Noise for Device #1234”

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: “E5500 Absolute Phase Noise Measurement.”

SCPI Compliance: Instrument Specific.

## 10 **FORMat Commands**

FORMat Command Introduction [184](#)

FORMat[:DATA] [185](#)



## **FORMat Command Introduction**

Use the FORMat command to set a data format for transferring numeric and array information. This data format is used for both command and response data by those commands that are specifically designated to be affected by the FORMat function.

The commands in this subsystem have the following command hierarchy:

FORMat[:DATA] (ASCii, length)

## FORMat[:DATA]

Specifies the format (ASCII) and number of significant digits for block data transferred across the GPIB. Only ASCII format is currently supported.

### Command Syntax

```
FORMat [:DATA] ASCii, <length>
  <length> ::= an integer (NRF data)
  Where <length>: number of significant digits
```

### Example

```
FORMat ASCii, 9
```

### Query syntax

```
FORMat?
```

### Return format

CHAR, Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ASCii,6

SCPI Compliance: Instrument Specific.

### Additional information

FORMat[:DATA] affects transfers initiated with the following commands:

- CALC:DATA?
- [SENSe:]DATA?

ASCII data consists of one line per data point separated by CR/LF. See CALC:DATA? and [SENSe:]DATA? pages for line format information.

## **10 FORMat Commands**

## 11 **INITiate Commands**

- INITiate Commands Introduction 188
- INITiate[:IMMEDIATE][:ALL] 189
- INITiate[:IMMEDIATE]:CALibrate 190
- INITiate[:IMMEDIATE]:MEASure 191



## **INITiate Commands Introduction**

Use the INITiate commands to control when measurement acquisition occurs.

The commands in this subsystem have the following command hierarchy:

- INITiate[:IMMediate][:ALL]
- INITiate[:IMMediate]:CALibrate
- INITiate[:IMMediate]:MEASure

Also see related PAUSE:... commands

## INITiate[:IMMediate][:ALL]

Initiates a system calibration and measurement.

### Command syntax

```
INITiate[:IMMediate] [:ALL]
```

### Example

```
INIT
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **INITiate[:IMMediate]:CALibrate**

Initiate system calibration.

#### **Command syntax**

```
INITiate[:IMMediate] :CALibrate
```

#### **Example**

```
INITiate:CALibrate
```

#### **Query syntax**

Command Only

#### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

#### **Additional information**

Calibration parameters are set using the CALibrate: tree.

## INITiate[:IMMediate]:MEASure

Initiate measurement only – no calibration. Used for repeat measurements. If the measurement definition changes a new calibration is required.

### Command syntax

```
INITiate[:IMMediate] :MEASure
```

### Example

```
INITiate:MEASure
```

### Query syntax

Command Only

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## **11 INITiate Commands**

## 12 **MMEMemory Commands**

MMEMemory:LOAD[:ALL] 195

MMEMemory:STORe 196



## **MMEMory Commands Introduction**

The MMEMory commands provide mass storage capabilities for the system.

The commands in this subsystem have the following command hierarchy:

- MMEMory:LOAD[:ALL] ("path\name.pnm")
- MMEMory:STORe[:ALL] ("path\name.pnm")

## MMEMORY:LOAD[:ALL]

Load a measurement definition and data file.

### Command syntax

```
MMEMORY:LOAD [:ALL] <"path\file_name.pnm">
<path\file_name.pnm> ::= quoted string (full or relative path and
filename)
```

### Example

```
MMEMORY:LOAD "Measfiles\Phase1.pnm"
```

### Attribute summary

Synchronization Required: none

\*RST State: NA

SCPI Compliance: Standard

### Additional information

Use the MMEMORY:STORE command to store a file to load with MMEMORY:LOAD.

Note that there is no format specification. This file is stored in a format (.pnm files) relevant only to the Phase Noise Graphical User Interface (Phase.exe) or SCPI clients

## **MMEMory:STORe**

Stores the current measurement definition and data to a file.

### **Command syntax**

```
MMEMory:STORe <“path\file_name.pnm”>
<path\file_name.pnm> :: = quoted string (full or relative path and
filename)
```

### **Example**

```
MMEMory:STORe “.\measurements\meas1.pnm”
```

### **Query syntax**

Command Only

### **Return format**

### **Attribute summary**

Synchronization Required: none

\*RST State: NA

SCPI Compliance: Standard

### **Additional information**

Use the MMEMory:LOAD command to load a file stored with MMEMory:STORe.

**NOTE**

that there is no format specification. This file is stored in a format relevant only to the Phase Noise GUI or SCPI clients (.pnm files).

## 13 **PAUSe Commands**

- PAUSe Commands Introduction 198
- PAUSe:ABORT:AUTO 199
- PAUSe:ADJust:LNAGain 200
- PAUSe:ADJust:VCOCenter 201
- PAUSe:CONNect 202
- PAUSe:CONTinue 203
- PAUSe:RETRy 204
- PAUSe:SPECial 205



## **PAUSe Commands Introduction**

The commands in this subsystem have the following command hierarchy:

- PAUSe:ABORt:AUTO (0 | OFF | 1 | ON)
- PAUSe:ADJust:LNAGain
- PAUSe:ADJust:VCOCenter
- PAUSe:CONNect (0 | OFF | 1 | ON)
- PAUSe:CONTinue
- PAUSe:RETRY
- PAUSe:SPECial

## PAUSE:ABORT:AUTO

Automatically abort a calibration or measurement if and when a pause event occurs.

### Command syntax

```
PAUSE:ABORT:AUTO <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
PAUSE:ABORT:AUTO OFF
```

### Query syntax

```
PAUSE:ABORT:AUTO?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Instrument Specific.

### Additional information

Pause events include PAUSE:CONNECT ON, PAUSE:SPECIAL and any other events which interrupt the progression of a calibration or measurement.

### PAUSE:ADJust:LNAGain

Adjust the nominal gain for the low noise amplifier in the test set after autorange when the LNA gain adjust pause point is enabled.

#### Command syntax

```
PAUSE:ADJust:LNAGain <number> [dB]  
  
<number> ::= a real number (NRf data)  
Accepts numeric input but snaps to nearest of the following values:  
14  
28  
42  
56
```

#### Example

```
PAUSE:ADJust:LNAGain 28
```

#### Query syntax

```
PAUSE:ADJust:LNAGain?
```

#### Return format

Real

#### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 42 dB

SCPI Compliance: Instrument Specific.

#### Additional information

[SENSe:]TSET:LNAGain:METHod PAUSE must be set for PAUSE:ADJust:LNAGain to be in effect.

Also see: [SENSe:]TSET:LNAGain:METHod

## PAUSE:ADJust:VCOCenter

Adjust the VCO tuning center voltage when paused.

### Command syntax

```
PAUSE:ADJust:VCOCenter <number> [dB]  
<number> ::= a real number (NRF data)
```

### Example

```
PAUSE:ADJust:VCOCenter .5
```

### Query syntax

```
PAUSE:ADJust:VCOCenter?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0 V

SCPI Compliance: Instrument Specific.

### Additional information

The Tune Voltage allows you to change the tune voltage. IF the tuning voltage exceeds 10% of the peak tuning range during system calibration, the phase noise software stops the procedure and informs the user that the source needs to be retuned before the measurement can begin.

## **PAUSE:CONNect**

Enable or disable the presentation of the connect diagram.

### **Command syntax**

```
PAUSE:CONNect <boolean>
<boolean> ::= OFF|0|ON|1
```

### **Example**

```
PAUSE:CONNect ON
```

### **Query syntax**

```
PAUSE:CONNect?
```

### **Return format**

```
Integer 0=OFF 1=ON
```

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

### **Additional information**

When enabled, the system will always stop at this fixed point and wait for an INITiate:PAUSE:CONTinue command before proceeding. A message will be placed in the message queue.

If PAUSE:ABORT:AUTO is ON and PAUSE:CONNect is ON the measurement or calibration will abort when the connect diagram is presented. Normally, this should be avoided.

## PAUSE:CONTINUE

Continue from a pause point.

### Command syntax

PAUSE:CONTINUE

### Example

PAUSE:CONT

### Query syntax

Command Only

### Attribute summary

Synchronization required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## **PAUSE:RETRY**

Retry the last operation prior to a pause point.

### **Command syntax**

PAUSE:RETRY

### **Query syntax**

Command Only

### **Example**

PAUSE:RETRY

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State:NA

SCPI Compliance: Instrument Specific.

## PAUSE:SPECial

Specify a branch to be taken following a pause point.

### Command syntax

PAUSE:SPECial <response>

<response> ::= a real number (NRf data)

limits: see discussion

### Query syntax

### Example

### Return format


### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

## 13 PAUSE Commands

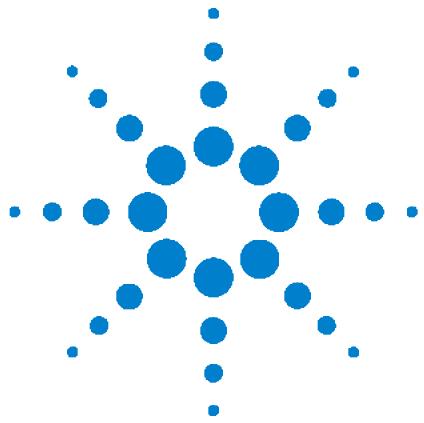

## 14 **SENSe Commands**

- SENSe Commands Introduction [209](#)
- [SENSe:]DATA? [211](#)
- [SENSe:]DATA:HEADER:POINTs? [212](#)
- [SENSe:]DCONverter:ATTenuator [213](#)
- [SENSe:]DCONverter:ATTenuator:AUTO [214](#)
- [SENSe:]DCONverter:ATTenuator:AUTO:IMMEDIATE [215](#)
- [SENSe:]DCONverter:BAND [216](#)
- [SENSe:]DCONverter:FREQuency [217](#)
- [SENSe:]DCONverter:IFFRquency? [218](#)
- [SENSe:]DCONverter:IFGain [219](#)
- [SENSe:]DCONverter:IFGain:AUTO [220](#)
- [SENSe:]DCONverter:IFGain:AUTO:IMMEDIATE [221](#)
- [SENSe:]DCONverter:L1BWidth [222](#)
- [SENSe:]DCONverter:L6BWidth [223](#)
- [SENSe:]DCONverter:LOPower [224](#)
- [SENSe:]DCONverter:LOSelect [225](#)
- [SENSe:]DCONverter:LOSelect:AUTO [226](#)
- [SENSe:]DCONverter:MEXT:BIAS [227](#)
- [SENSe:]DCONverter:MEXT:BIAS:STATe [228](#)
- [SENSe:]DCONverter:MMLO? [229](#)
- [SENSe:]DCONverter:PLO [230](#)
- [SENSe:]DCONverter:REFERENCE [231](#)
- [SENSe:]DCONverter:TSENSitivity? [232](#)
- [SENSe:]DCONverter:TUNE:PORT [234](#)
- [SENSe:]DETector:FREQuency [235](#)
- [SENSe:]DETector:SElect [236](#)
- [SENSe:]FFT:INPut:COUpling [238](#)
- [SENSe:]NOISe:BBGain [239](#)
- [SENSe:]NOISe:FFT [240](#)
- [SENSe:]NOISe:MEAStype [241](#)
- [SENSe:]NOISe:PULSed [242](#)
- [SENSe:]NOISe:QUADrature[:METHOD] [243](#)
- [SENSe:]RANGE:FFT:AVERage:MINimum [244](#)
- [SENSe:]RANGE:FFT:SEGTable [:MEASurement][:QUALity] [245](#)



[SENSe:]RANGE:OFFSet 246  
[SENSe:]RANGE:SWEPt:SEGTable [:MEASurement][:QUALity] 247  
[SENSe:]TSET:ATTenuator 248  
[SENSe:]TSET:ATTenuator:AUTO 249  
[SENSe:]TSET:LNAGain:METHod 252  
[SENSe:]TSET:LNAGain:MINimum 253  
[SENSe:]TSET:LPF 254  
[SENSe:]TSET:LPF:AUTO 255  
[SENSe:]TSET:PLL:ATTenuator 256  
[SENSe:]TSET:PLL:UNLock:IGNore 258

## SENSe Commands Introduction

The commands in this subsystem have the following command hierarchy:

- [:SENSe]:DATA?
- [:SENSe]:DATA:HEADER:POINTs?
- [:SENSe]:DCONverter:ATTenuator (0 to 35 dB in 5 dB steps)
- [:SENSe]:DCONverter:ATTenuator:AUTO (0 | OFF | 1 | ON)
- [:SENSe]:DCONverter:ATTenuator:AUTO:IMMEDIATE
- [:SENSe]:DCONverter:BAND (UWAVe | A | K | Q | U | V | W)
- [:SENSe]:DCONverter:FREQuency (value)
- [:SENSe]:DCONverter:IFFREQuency?
- [:SENSe]:DCONverter:IFGain (-10 to 45 dB in 5 dB steps)
- [:SENSe]:DCONverter:IFGain:AUTO (0 | OFF | 1 | ON)
- [:SENSe]:DCONverter:IFGain:AUTO:IMMEDIATE
- [:SENSe]:DCONverter:L1BWdth (value)
- [:SENSe]:DCONverter:L6BWdth (value)
- [:SENSe]:DCONverter:LOPower (value)
- [:SENSe]:DCONverter:LOSelect (value)
- [:SENSe]:DCONverter:LOSelect:AUTO (0 | OFF | 1 | ON)
- [:SENSe]:DCONverter:MEXT:BIAS (value)
- [:SENSe]:DCONverter:MEXT:BIAS:STATE (0 | OFF | 1 | ON)
- [:SENSe]:DCONverter:MMLO?
- [:SENSe]:DCONverter:PLO
- [:SENSe]:DCONverter:REFerence (value)
- [:SENSe]:DCONverter:TSENsitivity?
- [:SENSe]:DCONverter:TUNE:PORT (OFF | INTernal | FRONT | REAR)
- [:SENSe]:DETEctor:FREQuency (value)
- [:SENSe]:DETEctor:SElect (AUTO | EXT | LFR | HFR | UWAVe | TAM | TINoise | DCAM | DIAM)
- [:SENSe]:FFT:INPUT:COUPling (AC | DC)
- [:SENSe]:NOISE:BBGain (value)
- [:SENSe]:NOISE:FFT (EXTended | MULTiple)
- [:SENSe]:NOISE:MEAStype (ABS | RES | FM | AM | BBAN | NOTS)
- [:SENSe]:NOISE:PULsed (0 | OFF | 1 | ON)
- [:SENSe]:NOISE:QUADrature[:METHOD] (PSHifter | SOURce)

- [:SENSe]:RANGE:FFT:AVERage:MINimum (value)
- [:SENSe]:RANGE:FFT:SEGTable[:MEASurement][{:QUALity}] (NORMAl | FAST | ACCurate | CUSTom)
- [:SENSe]:RANGE:OFFSet (Start frequency, Stop frequency)
- [:SENSe]:RANGE:SWEPt:SEGTable[:MEASurement][{:QUALity}] (NORMAl | FAST | ACCurate | CUSTom)
- [:SENSe]:TSET:ATTenuator (value)
- [:SENSe]:TSET:ATTenuator:AUTO (0 | OFF | 1 | ON)
- [:SENSe]:TSET:DCBlock (0 | OFF | 1 | ON)
- [:SENSe]:TSET:LNAGain (value)
- [:SENSe]:TSET:LNAGain:METHod (AUTO | FIXed | PAUSe)
- [:SENSe]:TSET:LNAGain:MINimum (value)
- [:SENSe]:TSET:LPF (value)
- [:SENSe]:TSET:LPF:AUTO (0 | OFF | 1 | ON)
- [:SENSe]:TSET:PLL:ATTenuator (value)
- [:SENSe]:TSET:PLL:UNLock:IGNore (0 | OFF | 1 | ON)
- [:SENSe]:TVCO (REFerence | CARRier | DCONverter | INTernal)

## [SENSe:]DATA?

Retrieves the raw S-phi data for the user-defined measurement range.

### Command Syntax

Query Only

#### Query syntax

[SENSe : ] DATA?

#### Return format

Returns triples with each element separated by a comma and terminated by cr/lf. Each triple consists of the frequency, amplitude and spur flag.

Frequency, Amplitude, Spur\_Flag

Spur\_Flag: 1=spur 0=noise

#### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

#### Additional information

S-phi data corresponds to data displayed by DISPlay:GRAPH:TRANSform SDPF.

Returns one line per data point as indicated by [SENSe:]DATA:HEADER:POINts?. Number of significant digits for frequency and amplitude is controlled by FORMat[:DATA] command.

## [SENSe:]DATA:HEADer:POINTs?

Returns the number of data points which will be returned by [SENSe:]DATA?

### Command Syntax

Query Only

### Query syntax

[SENSe:] DATA:HEADer:POINTs?

### Return format

Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Standard

## [SENSe:]DCONverter:ATTenuator

Specify the amount of input attenuation for the downconverter.

### Command syntax

```
[SENSe:] DCONverter:ATTenuator <number> [dB]  
<number> ::= a real number (NRF data)  
Accepts numeric inputs, but snaps to nearest of the following values: 0,  
5, 10, 15, 20, 25, 30, 35
```

### Example

```
DCONverter:ATTenuator 15
```

### Query syntax

```
[SENSe:] DCONverter:ATTenuator?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0 dBm

SCPI Compliance: Instrument Specific.

### Additional information

This command is significant only if an Agilent N5507A downconverter is used. The N5507A is the only downconverter available with an input attenuator. The value specified here will be used by the system if autoranging has been disabled ([SENSe:]DCONverter:ATTenuator:AUTO OFF).

## [SENSe:]DCONverter:ATTenuator:AUTO

When enabled, the system will perform automatic autoranging of the downconverter input attenuator.

### Command syntax

```
[SENSe :] DCONverter:ATTenuator:AUTO <boolean>
<boolean> ::= OFF | 0 | ON | 1
```

### Example

```
DCONverter:ATTenuator:AUTO ON
```

### Query syntax

```
DCONverter:ATTenuator:AUTO?
```

### Return format

Integer 0=OFF, 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ON

SCPI Compliance: Instrument Specific.

### Additional information

If auto input attenuation is enabled, at the appropriate time in the measurement the measurement engine will instruct the downconverter to do an autorange immediate on the input attenuator. If auto is disabled, the value set by [SENSe:]DCONverter:ATTenuator will be used.

If both an Agilent N5500A OPT 001 and N5507A are in the system, and both attenuators have been set to AUTO, then the test set attenuator is autoranged first, then the downconverter attenuator, then the IF gain. That is, always perform autoranges in order from the beginning of the signal path, paying attention to the auto/manual switches set by the user. The philosophy is to never override a user's value if manual is selected.

## [SENSe:]DCONverter:ATTenuator:AUTO: IMMediate

Perform downconverter attenuator autorange.

### Command syntax

[SENSe:] DCONverter:ATTenuator:AUTO:IMMediate

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: n/a

SCPI Compliance: Instrument Specific.

### Additional information

Normally issued by the driver automatically. See  
[SENSe:]DCONverter:Attenuator:AUTO

## [SENSe:]DCONverter:BAND

Specify the input frequency band of the downconverter.

### Command syntax

```
[SENSe :] DCONverter:BAND UWAvE|A|K|Q|U|V|W
```

### Example

```
DCONverter:BAND K
```

### Query syntax

```
DCONverter:BAND?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: UWAVe

SCPI Compliance: Instrument Specific.

### Additional information

Selects either microwave or millimeter-wave mode. In millimeter mode an external harmonic mixer is used to convert the signal to a frequency within the downconverter's IF range.

## [SENSe:]DCONverter:FREQuency

Specify the downconverter input frequency.

### Command syntax

```
[SENSe:] DCONverter:FREQuency <number> [Hz | kHz | MHz | GHz]  
<number> ::= a real number (NRF data)
```

### Example

```
DCONverter:FREQuency 8E9
```

### Query syntax

```
DCONverter:FREQuency?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 10E9 Hz

SCPI Compliance: Instrument Specific.

## [SENSe:]DCONverter:IFFFrequency?

Query the IF frequency of the downconverter.

### Command Syntax

Query Only

### Query syntax

[SENSe:]DCONverter:IFFFrequency?

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

### Additional information

Displays the downconverter's IF frequency. When an Input Frequency is entered, the downconverter computes the IF frequency and displays it. The IF frequency can be changed by changing the LO Frequency. The new IF frequency will be calculated and displayed even if it is out of range. The IF frequency is automatically set when the Auto is selected.

## [SENSe:]DCONverter:IFGain

Specify the gain for the IF amplifier in the downconverter.

### Command syntax

```
[SENSe:] DCONverter:IFGain <number> [dB]  
<number> ::= a real number (NRF data)  
limits: -10:+45 in 5dB steps
```

### Example

```
DCONverter:IFGain
```

### Query syntax

```
DCONverter:IFGain?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0 dBm

SCPI Compliance: Instrument Specific.

## [SENSe:]DCONverter:IFGain:AUTO

Turn downconverter IF Gain auto ranging on or off.

### Command syntax

```
[SENSe:] DCONverter:IFGain:AUTO <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
DCONverter:IFGain:AUTO OFF
```

### Query syntax

```
DCONverter:IFGain:AUTO?
```

### Return format

Integer 0=OFF, 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ON

SCPI Compliance: Instrument Specific.

### Additional information

This command does not turn on or off an autoranging function in the downconverter. If autoranging is enabled, at the appropriate time in the measurement, the phase noise measurement software sends a command to the downconverter to have it do a one-time autorange.

The IF gain is automatically set by triggering a one-time autoranging when the Auto button is clicked. The downconverter autoranges the IF amplifier's gain by first setting the gain to its minimum (-10 dB) then stepping the gain up in 5 dB steps until the signal level at the IF amplifier's output is between 0 and +6 dBm.

## [SENSe:]DCONverter:IFGain:AUTO: IMMediate

Perform downconverter IF gain autorange.

### Command syntax

[SENSe:] DCONverter:IFGain:AUTO:IMMediate

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: n/a

SCPI Compliance: Instrument Specific.

### Additional information

Normally issued by the driver automatically. See  
[SENDe:]DCONverter:IFGain:AUTO

## [SENSe:]DCONverter:L1BWidth

Sets or queries the 100 MHz PLL bandwidth value.

### Command syntax

```
[SENSe:] DCONverter:L1BWidth <value>
<value> ::= a real number (NRf data)
```

Accepts numeric input but snaps to nearest of the following values:

- 25 Hz
- 53 Hz
- 126 Hz
- 300 Hz
- 650 Hz
- 1500 Hz
- 3600 Hz
- 10000 Hz

### Example

```
DCONverter:L1BWidth 300
```

### Query syntax

```
DCONverter:L1BWidth?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 3

SCPI Compliance: Instrument Specific.

## [SENSe:]DCONverter:L6BWidth

Specify the downconverter's 600 MHz PLL bandwidth.

### Command syntax

```
[SENSe:] DCONverter:L6BWidth <value>
<value> ::= a real number (NRf data)
```

Accepts numeric input but snaps to nearest of the following values:

- 4 kHz
- 10 kHz
- 17 kHz
- 30 kHz

### Example

```
DCONverter:L6BWidth 17E6
```

### Query syntax

```
DCONverter:L6BWidth?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 10E3

SCPI Compliance: standard

## [SENSe:]DCONverter:LOPower

Specify downconverter LO power.

### Command syntax

```
[SENSe:] DCONverter:LOPower <number> [dBm]  
<number> ::= a real number (NRF data)
```

### Example

```
DCONverter:LOPower 20
```

### Query syntax

```
DCONverter:LOPower?
```

### Return format

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 20 dBm

SCPI Compliance: Instrument Specific.

## [SENSe:]DCONverter:LOSelect

Set the frequency to steer the YIG to one of the SRD comb frequencies.

### Command syntax

```
[SENSe:] DCONverter:LOSelect <frequency> [<frequency_suffix>]  
<frequency>       ::= a real number (NRF data)  
<frequency_suffix> ::= MHz | GHz
```

### Example

```
DCONverter:LOSelect 1.5E9
```

### Query syntax

```
DCONverter:LOSelect?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1E9 Hz

SCPI Compliance: Instrument Specific.

## [SENSe:]DCONverter:LOSelect:AUTO

Turn downconverter frequency auto selection on or off.

Command syntax

```
[SENSe:] DCONverter:LOSelect:AUTO <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
DCONverter:LOSelect:AUTO OFF
```

### Query syntax

```
DCONverter:LOSelect:AUTO?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ON

SCPI Compliance: Instrument Specific.

## [SENSe:]DCONverter:MEXT:BIAS

Sets or queries the external mixer DC bias current.

### Command syntax

```
[SENSe:] DCONverter:MEXT:BIAS <number> [mA]  
<number> ::= a real number (NRF data)  
limits: -10:+10
```

### Example

```
DCONverter:MEXT:BIAS.002
```

### Query syntax

```
DCONverter:MEXT:BIAS?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0.0 mA

SCPI Compliance: Instrument Specific.

### Additional information

The millimeter mixer is external to the downconverter and may require DC bias for proper operation with odd harmonics of the LO. The DC bias current will be present at the signal input of the downconverter when enabled.

## [SENSe:]DCONverter:MEXT:BIAS:STATE

Turns the external mixer bias voltage ON|OFF.

### Command syntax

```
[SENSe:] DCONverter:MEXT:BIAS:STATE <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
DCONverter:MEXT:BIAS:STATE ON
```

### Query syntax

```
DCONverter:MEXT:BIAS:STATE?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

### Additional information

The millimeter mixer is external to the downconverter and may require DC bias for proper operation with odd harmonics of the LO. The DC bias voltage will be present at the signal input of the downconverter when enabled.

## [SENSe:]DCONverter:MMLO?

Query the external Millimeter mixer's LO frequency.

### Command Syntax

Query Only

### Query syntax

[SENSe:]DCONverter:MMLO?

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: N\A

SCPI Compliance: Instrument Specific.

## [SENSe:]DCONverter:PLO

Peak Downconverter LO.

### **Command syntax**

[SENSe:]DCONverter:PLO

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

### **Additional information**

Peak LO command - N5507A Option H16 version. Normally issued by the driver automatically. May also be issued by downconverter asset control panel.

## [SENSe:]DCONverter:REFerence

Select downconverter reference oscillator(s)

### Command syntax

```
[SENSe:] DCONverter:REFerence <number>
<value> ::= a real number (NRF data)
```

Accepts numeric input but snaps to nearest of the following values:

- 10 E6
- 100 E6
- 600 E6

### Example

```
[SENSe:]DCONverter:REFerence 100E6
```

### Query syntax

```
[SENSe:]DCONverter:REFerence?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 10.000000 E+6

SCPI Compliance: Instrument Specific.

### Additional information

- 10E6 selects the 10, 100, and 600 MHz oscillators
- 100E6 selects the 100 and 600 MHz oscillators
- 600E6 selects the 600 MHz oscillator

## [SENSe:]DCONverter:TSENsitivity?

Returns the downconverter tuning sensitivity.

### Command Syntax

Query Only

### Query syntax

[SENSe:]DCONverter:TSENsitivity?

### Return format

- 0
- 0.05
- 1
- 20

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1

SCPI Compliance: Instrument Specific.

### Additional information

The response to this query is controlled by the setting of these commands:

- [SENSe:]DCONverter:TUNE:PORT
- [SENSe:]DCONverter:REFerence

0 corresponds to: 10MHz No Tune, All oscillators phase locked, 10 MHz tune input grounded.

- [SENSe:]DCONverter:TUNE:PORT OFF
- [SENSe:]DCONverter:REFerence 10E6

0.05 corresponds to: All oscillators phase locked, 10 MHz tune enabled.

- [SENSe:]DCONverter:TUNE:PORT INTernal|FRONT|REAR
- [SENSe:]DCONverter:REFerence 10E6

1 corresponds to: 10 MHz out of chain, 600 MHz phase locked to 100 MHZ, 100 MHz tune enabled.

- [SENSe:]DCONverter:TUNE:PORT INTernal|FRONT|REAR
- [SENSe:]DCONverter:REFerence 100E6

20 corresponds to: 10 MHz and 100 MHz out of chain, 600 MHz tune enabled.

- [SENSe:]DCONverter:TUNE:PORT INTernal|FRONT|REAR
- [SENSe:]DCONverter:REFerence 600E6

For more information, refer to the 70427A/70428A Microwave Downconverter / Microwave Source User's Guide.

## [SENSe:]DCONverter:TUNE:PORT

Select downconverter tuning port

### Command syntax

```
[SENSe:] DCONverter:TUNE:PORT INTERNAL|OFF|FRONT|REAR
```

### Example

```
DCONverter:TUNE:PORT OFF
```

### Query syntax

```
[SENSe:] DCONverter:TUNE:PORT?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

## [SENSe:]DETector:FREQuency

Specify detector input frequency.

### Command syntax

```
[SENSe:] DETector:FREQuency <number>
<number> ::= a real number (NRf data)
```

### Example

```
DETector:FREQuency 600E6
```

### Query syntax

```
DETector:FREQuency?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 500E6 Hz

SCPI Compliance: Instrument Specific.

### Additional information

The Detector Input Frequency is the frequency of the input signal connected to the system's phase detector. The Detector Input Frequency is used to:

Select the appropriate Low Pass Filter (LPF) in the phase noise system. For frequencies < 95 MHz, the test system enables the 2 MHz LPF to eliminate feed through of the fundamental signal and the additive products out of the phase detector. When the 2 MHz LPF is enabled, the maximum offset frequency the test system can measure is 2 MHz.

Set the frequency of the reference source when the reference source is under system control.

## [SENSe:]DETector:SElect

Specify the input for the detector.

### Command syntax

```
[SENSe :] DETector:SElect AUTO|EXTernal|LFREquency|HFREquency  
|UWAVE|TAM|TINoise|DCAM
```

### Example

```
DETector:SElect LFR
```

### Query syntax

```
DETector:SElect?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: AUTO

SCPI Compliance: Instrument Specific.

### Additional information

- AUTO specifies auto selection of the detector. Note that this will auto select only between the LFREquency, HFREquency, and UWAVE detectors based upon detector input frequency.
- LFREquency selects the low frequency phase detector.
- HFREquency selects the high frequency phase detector.
- UWAVE selects the microwave phase detector.
- TAM selects the test set AM detector.
- DCAM selects the downconverter AM detector.
- TINoise selects the test set internal calibration noise source.

Connect diagram implications:

- AUTO - one of the two REF INPUT ports of test set is connected.
- EXTernal or TAM - the NOISE INPUT port of the test set is connected.

- LFREference or HFREference - REF INPUT 500kHz-1600MHz is connected.
- UWAVE - REF INPUT 1.2-26.5 REF INPUT is connected.
- DCAM - SIGNAL INPUT for the downconverter (note that there is no AM detector in the Agilent 70422A).

## [SENSe:]FFT:INPut:COUPling

Selects AC or DC coupling for the FFT Analyzer Input Coupling.

### Command syntax

[SENSe:] FFT:INPut:COUPling AC|DC

### Example

FFT:INPut:COUPling DC

### Query syntax

FFT:INPut:COUPling?

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: AC

SCPI Compliance: Instrument Specific.

## [SENSe:]NOISe:BBGain

Specify the compensation for an external amplifier's gain.

### Command syntax

```
[SENSe:]NOISe:BBGain <number> [dB]
<number> ::= a real number (NRF data)
```

### Example

```
NOISe:BBGain 10
```

### Query syntax

```
NOISe:BBGain?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0 dBm

SCPI Compliance: Instrument Specific.

### Additional information

This is used when an amplifier is inserted between the DUT (device under test) and the 'Noise' input to the test set and the engineer wants the theoretical noise of the amplifier to be accounted for and removed from the measurement results.

This function is used to offset the plotted measurement data. It compensates for any additional amplifiers or attenuators being used when making the measurement.

- Offsets > 0 compensate for known gains.
- Offsets < 0 compensate for known losses.

## [SENSe:]NOISe:FFT

Specify whether multiple time samples or an extended time sample should be used by the FFT analyzer.

### Command syntax

```
[SENSe:] NOISe:FFT EXTended|MULTiple
```

### Query syntax

```
NOISe:FFT MULT
```

### Example

```
NOISe:FFT?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: MULTiple

SCPI Compliance: Instrument Specific.

### Additional information

EXTended refers to the ability of the E1430 Digitizer to record a single extended time segment from which multiple FFT's are derived. This feature should greatly reduce measurement time. MULTiple is the current method of recording smaller time segments, which produce many FFT's for averaging.

## [SENSe:]NOISE:MEAStype

Specify the measurement type.

### Command syntax

```
[SENSe:] NOISE:MEAStype
ABSolute|RESidual|FMDiscriminator|AM|BBAND|NOTSet
```

### Example

```
NOISE:MEAStype BBAND
```

### Query syntax

```
NOISE:MEAStype?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ABSolute

SCPI Compliance: Instrument Specific.

### Additional information

- ABSolute. .... Phase Noise using a Phase Locked Loop
- RESidual. .... Phase Noise without using a Phase Locked Loop
- FMDiscriminator. .... Phase Noise using an FM Discriminator
- AM. .... AM Noise Measurement
- BBAND. .... Base Band Noise Measurement
- NOTSetBase Band Noise Measurement without using the Test Set

## [SENSe:]NOISe:PULSed

Turn source signal pulsed mode on or off.

### Command syntax

```
[SENSe:]NOISe:PULSed <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
NOISe:PULSed?
```

### Query syntax

```
NOISe:PULSed ON
```

### Return format

```
Integer 0=OFF 1=ON
```

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

### Additional information

The FREQuency mode is always CW and therefore does not have to be specified. The sources can be pulsed, however.

## [SENSe:]NOISe:QUADrature[:METHOD]

Specify the method used to achieve quadrature for a residual measurement.

### Command syntax

```
[SENSe:] NOISe:QUADrature [:METHOD] PSHifter|SOURce
```

### Example

```
NOISe:QUADrature PSH
```

### Query syntax

```
NOISe:QUADrature?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: SOURce

SCPI Compliance: Instrument specific

## [SENSe:]RANGE:FFT:AVERage:MINimum

Specify the minimum number of averages for the measurement range.

### Command syntax

```
[SENSe:] RANGE:FFT:AVERage:MINimum <number>
<number> ::= a real number (NRF data)
```

### Example

```
RANGE:FFT:AVERage:MINimum 5
```

### Query syntax

```
RANGE:FFT:AVERage:MINimum?
```

### Return format

Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 4

SCPI Compliance: Instrument Specific.

### Additional information

The minimum number of averages defined for the measurement determines the minimum number of noise level measurements the phase noise software will make for each segment of the specified offset range. The phase noise software actually takes more averages if the minimum number of averages specified in the segment table is greater than the number of averages specified here.

## [SENSe:]RANGE:FFT:SEGTable[:MEASurement][:QUALity]

Specify which FFT segment table to use for the specified range.

### Command syntax

```
[SENSe:] RANGE:FFT:SEGTable [:MEASurement] [:QUALity]
NORMAL | FAST | HRESolution | CUSTOM
```

### Example

```
RANGE:FFT:SEGTable:MEASurement:QUALity HRESolution
```

### Query syntax

```
RANGE:FFT:SEGTable:MEASurement:QUALity?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NORMAL

SCPI Compliance: Instrument Specific.

### Additional information

- NORMAL
- FAST - quickest, but the least accurate
- HRESolution - slowest and most accurate
- CUSTOM- speed and accuracy are user defined

## [SENSe:]RANGE:OFFSet

Specify the offsets for a measurement range.

Command syntax  
[SENSe:] RANGE:OFFSet <start\_offset> [<frequency\_suffix>]  
                         , <stop\_offset> [<frequency\_suffix>]  
<start\_offset>       ::= a real number (NRF data)  
<stop\_offset>     ::= a real number (NRF data)  
<frequency\_suffix> ::= Hz | kHz | MHz | GHz

### Example

```
SENSe:RANGE:OFFSet 10Hz,500Hz
```

### Query syntax

```
SENSe:RANGE:OFFSet?
```

### Return format

Real, Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1Hz,100MHz

SCPI Compliance: Instrument Specific.

## [SENSe:]RANGE:SWEPt:SEGTable[:MEASurement][:QUALity]

Specify which Swept segment table to use for the specified range.

### Command syntax

```
[SENSe:] RANGE:SWEPt:SEGTable[:MEASurement][:QUALity]
NORMAl | FAST | HRESolution | CUSTOM
```

### Example

```
RANGE:SWEPt:SEGTable:MEASurement:QUALity HRESolution
```

### Query syntax

```
RANGE:SWEPt:SEGTable:MEASurement:QUALity?
```

### Return format

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NORMAl

SCPI Compliance: Instrument Specific.

### Additional information

- NORMAl
- FAST - quickest, but the least accurate
- HRESolution - slowest and most accurate
- CUSTOM- speed and accuracy are user defined

## [SENSe:]TSET:ATTenuator

Specify the amount of attenuation applied at the signal input of the test set.

### Command syntax

```
[SENSe:] TSET:ATTenuator <number> [dB]  
<number> ::= a real number (NRf data)
```

Accepts numeric input but snaps to nearest of the following values:

0, 5, 10, 15, 20, 25, 30, 35

### Example

```
TSET:ATTenuator 15
```

### Query syntax

```
TSET:ATTenuator?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0 dBm

SCPI Compliance: Instrument Specific.

### Additional information

This command is significant only if a N5500A OPT 001 test set is used. The N5500A OPT 001 is the only test set available with an input attenuator.

## [SENSe:]TSET:ATTenuator:AUTO

When enabled, the system will perform automatic autoranging of the test set input attenuator.

### Command syntax

```
[SENSe:] TSET:ATTenuator:AUTO <boolean>
<boolean> ::= OFF | 0 | ON | 1
```

### Example

```
TSET:ATTenuator:AUTO OFF
```

### Query syntax

```
TSET:ATTenuator:AUTO?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ON

SCPI Compliance: Instrument Specific.

### Additional information

This command is significant only if an N5500A OPT 001 test set is used. The N5500A OPT 001 is the only test set available with an input attenuator.

If auto input attenuation is enabled, at the appropriate time in the measurement the measurement engine will instruct the test set to do an autorange immediate on the input attenuator. If auto is disabled, the value set by [SENSe:]TSET:ATTenuator will be used.

If both a N5500A OPT 001 and an N5507A are in the system, and both attenuators have been set to AUTO, then the test set attenuator is autoranged first, then the downconverter attenuator, then the IF gain. That is, always perform autoranges in order from the beginning of the signal path, paying attention to the auto/manual switches set by the user. The philosophy is to never override a user's value if manual is selected.

## [SENSe:]TSET:DCBLock

Turn the DC high-pass filter ON or OFF.

### Command syntax

```
[SENSe:] TSET:DCBLock <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
TSET:DCBLock ON
```

### Query syntax

```
TSET:DCBLock?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Instrument Specific.

### Additional information

Check the DC block when performing AM noise measurements. The N5500A Phase Noise Test Set must be DC blocked when using its Noise Input. The test set will not tolerate more than +/- mV DC input without overloading the Low Noise Amplifier (LNA).

This filter is marked “AM BLOCK” on the block diagrams. It follows the phase detector LPF.

## [SENSe:]TSET:LNAGain

Specify the nominal gain for the low noise amplifier in the test set.

### Command syntax

```
[SENSe:] TSET:LNAGain <number> [dB]  
<number> ::= a real number (NRf data)
```

Accepts numeric inputs, but snaps to nearest following values:

14, 28, 42, 56

### Example

```
TSET:LNAGain 28
```

### Query syntax

```
TSET:LNAGain?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 42 dB

SCPI Compliance: Instrument Specific.

### Additional information

[SENSe:]TSET:LNAGain:METHod FIXed must be set for TSET:LNAGain to be in effect.

## [SENSe:]TSET:LNAGain:METHod

Specify the method for applying LNA gain.

### Command syntax

```
[SENSe:] TSET:LNAGain:METHod AUTO|FIXed|PAUSE
```

### Example

```
TSET:LNAGain:METHod FIXed
```

### Query syntax

```
TSET:LNAGain:METHod?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: AUTO

SCPI Compliance: Instrument Specific.

### Additional information

- AUTO = Auto Gain performs a one-time autoranging of the test set's LNA gain. The minimum gain selected is limited by [SENSe:]TSET:LNAGain:MINimum
- FIXed = use value set by [SENSe:]TSET:LNAGain
- PAUSE = Same as AUTO but generates a pause point after setting the gain.

## [SENSe:]TSET:LNAGain:MINimum

Specify the LNA gain minimum limit.

### Command syntax

```
[SENSe:] TSET:LNAGain:MINimum <number> [dB]  
<number> ::= a real number (NRf data)  
limits: 14|28|42|56
```

### Example

```
TSET:LNAGain:MINimum 28
```

### Query syntax

```
TSET:LNAGain:MINimum?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 14 dBm

SCPI Compliance: Instrument Specific.

### Additional information

Only applies if [SENSe:]TSET:LNAGain:METHod = AUTO | PAUSE

## [SENSe:]TSET:LPF

Specify the cutoff frequency for the input LPF of the Test Set.

### Command syntax

```
[SENSe:]TSET:LPF <value>
<value> ::= a real number (NRf data)
```

Accepts numeric input but snaps to nearest of the following values:

- 20 kHz
- 200 kHz
- 2 MHz
- 20 MHz
- 100 MHz

### Query syntax

```
TSET:LPF?
```

### Example

```
TSET:LPF 2E6
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State:

SCPI Compliance: Instrument Specific.

### Additional information

Requires [SENSe:]TSET:LPF:AUTO OFF

The lowpass filters follow the RF phase detectors (LF & HF) in the signal path. The block diagram shows the first filter as a 140 MHz LPF, but the system can only measure up to a 100 MHz offset, so functionally, this filter is a 100 MHz LPF. From the user's standpoint and from the measurement engine's standpoint, this is a 100 MHz LPF.

## [SENSe:]TSET:LPF:AUTO

Turn test set LPF automatic selection on or off.

### Command syntax

```
[SENSe:] TSET:LPF:AUTO <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
TSET:LPF:AUTO
```

### Query syntax

```
TSET:LPF:AUTO?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: ON

SCPI Compliance: Instrument Specific.

### Additional information

When LPF automatic selection is ON, the system will select an appropriate cutoff frequency based on the measurement type and the detector input frequency. When LPF automatic selection is OFF, the system will use the cutoff specified by [SENSe:]TSET:LPF.

## [SENSe:]TSET:PLL:ATTenuator

Specify the attenuation setting for the PLL input attenuator of the test set.

### Command syntax

```
[SENSe:] TSET:PLL:ATTenuator <enum> [dB]  
<enum>      ::= a real number (NRF data)
```

Accepts numeric input but snaps to nearest of the following values:

- 0.00 dB
- 6.28 dB
- 12.16 dB
- 18.12 dB
- 24.18 dB
- 30.48 dB
- 36.41 dB
- 42.43 dB

### Query syntax

```
TSET:PLL:ATTenuator?
```

### Example

```
TSET:PLL:ATTenuator 12.16
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 1

SCPI Compliance: Instrument Specific.

### Additional information

The PLL integrator attenuation can be switched in to provide for narrower voltage tune ranges.

The PLL input attenuator is the programmable attenuator located in front of the integrator on the PLL board. The associated test set command for this parameter is CTS:PLL:ATT3.

This attenuator changes the loop gain without affecting the drift tracking range (since it is ahead of the integrator). It has some significant effects on the ability to acquire lock under some conditions.

The direct affect from the user's point of view is on the loop bandwidth, but it is not necessarily a monotonic reduction of loop bandwidth (there are some sawteeth in the curve), and it takes some trial and error to figure out the optimal setting.

## [SENSe:]TSET:PLL:UNLock:IGNore

If ON, ignore PLL Unlocked errors and continued with the measurement.

### Command syntax

```
[SENSe:] TSET:PLL:UNLock:IGNore <boolean>
```

### Query syntax

```
TSET:UNLock:IGNore OFF
```

### Example

```
TSET:UNL:IGN?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none  
Preset (\*RST) State:OFF  
SCPI Compliance: Instrument Specific.

### Additional information

## [SENSe:]TVCO

Specifies where the tune voltage output is connected to.

### Command syntax

```
[SENSe:] TVCO REference|CARRier|DCONverter|INTernal
```

### Query syntax

```
SENSe:TVCO?
```

### Example

```
SENSe:TVCO DCONverter
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: REference

SCPI Compliance: Instrument Specific.

### Additional information

- REference specifies that the tune voltage output is connected to the Modulation Input of the reference source.
- CARRier specifies that the tune voltage output is connected to the Modulation Input of the carrier source.
- DCONverter specifies that the tune voltage output is connected to the Voltage Control Input port of the downconverter
- INTernal specifies that the tune voltage is routed internally to the test



## 15 **SOURce Commands**

- [SOURce Commands Introduction](#) 262
- [SOURce:CALibration:FM\[:DEViation\]](#) 263
- [SOURce:CALibration:FM:INTERNAL: FREQuency](#) 264
- [SOURce:CALibration:POWer \[:LEVel|AMPLitude\]](#) 266
- [SOURce:CARRier:FREQuency\[:CW|FIXed\]](#) 267
- [SOURce:CARRier:POWer \[:LEVel|AMPLitude\]](#) 268
- [SOURce:REFerence:FREQuency:DIVisor](#) 269
- [SOURce:REFerence:FREQuency:MULTiplier](#) 270
- [SOURce:REFerence:POWer \[:LEVel|AMPLitude\]](#) 271
- [SOURce:RESidual:FREQuency\[:CW | FIXed\]](#) 272
- [SOURce:RESidual:FREQuency:CALCulate](#) 273
- [SOURce:RESidual:FREQuency:DETector: COUPled](#) 274
- [SOURce:REFerence:FREQuency:DIVisor](#) 276
- [SOURce:RESidual:FREQuency:MULTiplier](#) 277
- [SOURce:RESidual:POWer \[:LEVel|AMPLitude\]](#) 278



## SOURce Commands Introduction

The SOURce subsystem is used to control source frequency and power parameters.

- SOURce:CALibration:FM[:DEViation] (value)
- SOURce:CALibration:FM:INTERNAL:FREQuency (value)
- SOURce:CALibration:FREQuency[:CW|FIXED] (value)
- SOURce:CALibration:POWer[:LEVel|AMPLitude] (value)
- SOURce:CARRier:FREQuency[:CW|FIXED] (value)
- SOURce:CARRier:POWer[:LEVel|AMPLitude] (value)
- SOURce:REFerence:FREQuency:DIVisor
- SOURce:REFerence:FREQuency:MULTiplier
- SOURce:REFerence:POWer[:LEVel|AMPLitude] (value)
- SOURce:RESidual:FREQuency[:CW|FIXED] (value)
- OURce:RESidual:FREQuency:CALCulate
- SOURce:RESidual:FREQuency:DETector:COUPled
- SOURce:RESidual:FREQuency:DIVisor
- SOURce:RESidual:FREQuency:MULTiplier
- SOURce:RESidual:POWer[:LEVel]|AMPLitude] (value)

## SOURce:CALibration:FM[:DEViation]

Specify the calibration source's modulation deviation of a FM signal.

### Command syntax

```
SOURce:CALibration:FM[:DEViation] <number> <frequency_suffix>
<number>      ::= a real number (NRF data)
<frequency_suffix> ::= Hz | kHz | MHz | GHz
```

### Example

```
SOURce:CALibration:FM 8E3
```

### Query syntax

```
SOURce:CALibration:FM?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 10 kHz

SCPI Compliance: Instrument Specific.

## **SOURce:CALibration:FM:INTernal: FREQuency**

Specify the calibration source's FM frequency.

### **Command syntax**

```
SOURce:CALibration:FM:INTernal:FREQuency <number>
<frequency_suffix>
<number>           ::= a real number (NRF data)
<frequency_suffix> ::= Hz|kHz|MHz|GHz
```

### **Example**

```
SOURce:CALibration:FM:INTernal:FREQuency?
```

### **Query syntax**

```
SOURce:CALibration:FM:INTernal:FREQuency 1.5E3
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 10 kHz

SCPI Compliance: Instrument Specific.

## SOURce:CALibration:FREQuency[:CW | FIXed]

Specify the calibration source frequency.

### Command syntax

```
SOURce:CALibration:FREQuency[:CW|FIXed] <number>
[<frequency_suffix>]
<number>      ::= a real number (NRF data)
<frequency_suffix> ::= Hz|kHz|MHz|GHz
```

### Example

```
SOURce:CALibration:FREQuency 600e6
```

### Query syntax

```
SOURce:CALibration:FREQuency?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 500 MHz

SCPI Compliance: Instrument Specific.

## **SOURce:CALibration:POWer [:LEVel | AMPLitude]**

Specify the calibration source power.

### **Command syntax**

```
SOURce:CALibration:POWer[:LEVel] [:AMPLitude] <number> [dBm]  
<number> ::= a real number (NRf data)
```

### **Example**

```
SOURce:CALibration:POWer 0
```

### **Query syntax**

```
SOURce:CALibration:POWer?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: +10 dBm

SCPI Compliance: Instrument Specific.

## SOURce:CARRier:FREQuency[:CW|FIXed]

Specify the carrier source frequency.

### Command syntax

```
SOURce:CARRier:FREQuency[:CW|FIXed] <number>
[<frequency_suffix>]
<number>       ::= a real number (NRF data)
<frequency_suffix> ::= Hz|kHz|MHz|GHz
```

### Example

```
SOURce:CARRier:FREQuency 10 GHz
```

### Query syntax

```
SOURce:CARRier:FREQuency?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 500 MHz

SCPI Compliance: Instrument Specific.

## SOURCE:CARRIER:POWER [:LEVEL | AMPLITUDE]

Specify the carrier source power.

### Command syntax

```
SOURCE:CARRIER:POWER[:LEVEL][:AMPLITUDE] <number> [dBm]  
<number> ::= a real number (NRF data)
```

### Example

```
SOURCE:CARRIER:POWER 10
```

### Query syntax

```
SOURCE:CARRIER:POWER?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: +10 dBm

SCPI Compliance: Instrument Specific.

### Additional information

The carrier power is the input power to the test set or the downconverter. The power must meet the minimum requirements of the test set's Signal Input.

## SOUrce:REFerence:FREQuency:DIVisor

Specify the reference source power.

### Command syntax

```
SOUrce:REFerence:FREQuency:DIVisor <number>
<number> ::= a real number (NRF data)
```

### Example

```
SOUrce:REFerence:FREQuency:DIVisor 3.0
```

### Query syntax

```
SOUrce:REFerence:FREQuency:DIVisor?
```

### Return format

Real

### Attribute summary

Synchronization Required: none  
Preset (\*RST) State: 1.0  
SCPI Compliance: Instrument Specific.

### Additional information

The Reference Source frequency is set to:

SENSE:DETector:FREQuency \*  
(SOUrce:REFerence:FREQuency:MULTiplier / SOUrce:REFerence:  
FREQuency:DIVisor)

## SOURCE:REFERENCE:FREQUENCY:MULTIPLIER

Specify the reference source power.

### Command syntax

```
SOURCE:REFERENCE:FREQUENCY:MULTIPLIER <number>
<number> ::= a real number (NRF data)
```

### Example

```
SOURCE:REFERENCE:FREQUENCY:MULTIPLIER 2.0
```

### Query syntax

```
SOURCE:REFERENCE:FREQUENCY:MULTIPLIER?
```

### Return format

Real

### Attribute summary

Synchronization Required: none  
Preset (\*RST) State: 1.0  
SCPI Compliance: Instrument Specific.

### Additional information

The Reference Source frequency is set to:

SENSE:DETECTOR:FREQUENCY \*  
(SOURCE:REFERENCE:FREQUENCY:MULTIPLIER / SOURCE:REFERENCE:  
FREQUENCY:DIVISOR)

## SOUrce:REFerence:POWeR [:LEVel | AMPLitude]

Specify the reference source power.

### Command syntax

```
SOUrce:REFerence:POWeR[:LEVel][:AMPLitude] <number> [dBm]  
<number> ::= a real number (NRf data)
```

### Example

```
SOUrce:REFerence:POWeR 10
```

### Query syntax

```
SOUrce:REFerence:POWeR?
```

### Return format

Real

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: +16 dBm

SCPI Compliance: Instrument Specific.

### Additional information

The reference source power is the reference input power to the test set. The power must meet the minimum requirements of the test set's Reference Input.

## **SOURce:RESidual:FREQuency[:CW | FIXed]**

Specify the residual source frequency.

### **Command syntax**

```
SOURce:RESidual:FREQuency[:CW|FIXed] <number>
[<frequency_suffix>]
<number> ::= a real number (NRF data)
<frequency_suffix> : : = Hz|kHz|MHz|GHz
```

### **Example**

```
SOURce:RESidual:FREQuency:CW 1E6
```

### **Query syntax**

```
SOURce:RESidual:FREQuency?
```

### **Return format**

Real

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: 500 MHz

SCPI Compliance: Instrument Specific.

## SOUrce:RESidual:FREQuency:CALCulate

When enabled, the Residual source frequency is coupled to the Carrier frequency.

### Command syntax

```
SOUrce:RESidual:FREQuency:CALCulate <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
SOUrce:RESidual:FREQuency:CALCulate OFF
```

### Query syntax

```
SOUrce:RESidual:FREQuency:CALCulate?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none  
 Preset (\*RST) State: ON  
 SCPI Compliance: Instrument Specific.

### Additional information

When SOUrce:RESidual:FREQuency:CALCulate is set to ON (the default) the Residual source frequency is automatically set based on the Carrier frequency and the Residual source Multiplier and Divisor. The following equation shows the relationship between the Carrier and Residual frequency, and the Multiplier and Divisor:

$$\text{Carrier} = \text{Residual} * (\text{Multiplier} / \text{Divisor})$$

Thus, for a given Carrier frequency, the Residual source is automatically set as follows:

$$\text{Residual} = \text{Carrier} / (\text{Multiplier} / \text{Divisor})$$

When SOUrce:RESidual:FREQuency:CALCulate is set to OFF, the Residual source frequency may be set independently of the Carrier frequency.

Also See:

- SOUrce:RESidual:FREQuency
- SOUrce:RESidual:FREQuency:DIVisor
- SOUrce:RESidual:FREQuency:MULTiplier

## SOURce:RESidual:FREQuency:DETector: COUPled

When enabled, the Residual source frequency is coupled to the Carrier frequency.

### Command syntax

```
SOURce:RESidual:FREQuency:DETector:COUPled <boolean>
<boolean> ::= OFF|0|ON|1
```

### Example

```
SOURce:RESidual:FREQuency:DETector:COUPled OFF
```

### Query syntax

```
SOURce:RESidual:FREQuency:DETector:COUPled?
```

### Return format

Intriguer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none  
 Preset (\*RST) State: ON  
 SCPI Compliance: Instrument Specific.

### Additional information

When SOURce:RESidual:FREQuency:DETector:COUPled is set to ON (the default) the Residual source frequency is automatically set based on the Carrier frequency and the Residual source Multiplier and Divisor. The following equation shows the relationship between the Carrier and Residual frequency, and the Multiplier and Divisor:

$$\text{Carrier} = \text{Residual} * (\text{Multiplier} / \text{Divisor})$$

Thus, for a given Carrier frequency, the Residual source is automatically set as follows:

$$\text{Residual} = \text{Carrier} / (\text{Multiplier} / \text{Divisor})$$

When SOURce:RESidual:FREQuency:DETector:COUPled is set to OFF, the Residual source frequency may be set independently of the Carrier frequency.

Also See:

SOURce:RESidual:FREQuency  
SOURce:RESidual:FREQuency:DIVisor  
SOURce:RESidual:FREQuency:MULTiplier

## SOURce:REFerence:FREQuency:DIVisor

Specify the residual source divisor.

### Command syntax

```
SOURce:RESidual:FREQuency:DIVisor <number>
<number> ::= a real number (NRF data)
```

### Example

```
SOURce:RESidual:FREQuency:DIVisor 3
```

### Query syntax

```
SOURce:RESidual:FREQuency:DIVisor?
```

### Return format

Real

### Attribute summary

Synchronization Required: none  
 Preset (\*RST) State: 1  
 SCPI Compliance: Instrument Specific.

### Additional information

The value of this parameter is only applied when SOURce:RESidual:FREQuency:DETector:COUPled is set to ON (the default). When this is true, the following equation shows the relationship between the Carrier and Residual frequency and Multiplier and Divisor:

$$\text{Carrier} = \text{Residual} * (\text{Multiplier} / \text{Divisor})$$

Thus, for a given Carrier frequency, the Residual source is automatically set as follows:

$$\text{Residual} = \text{Carrier} / (\text{Multiplier} / \text{Divisor})$$

## SOUrce:RESidual:FREQuency:MULTiplier

Specify the Residual source multiplier.

### Command syntax

```
SOUrce:RESidual:FREQuency:MULTiplier <number>
<number> ::= a real number (NRF data)
```

### Example

```
SOUrce:RESidual:FREQuency:MULTiplier 2
```

### Query syntax

```
SOUrce:RESidual:FREQuency:MULTiplier?
```

### Return format

Real

### Attribute summary

Synchronization Required: none  
 Preset (\*RST) State: +16 dBm  
 SCPI Compliance: Instrument Specific.

### Additional information

The value of this parameter is only applied when SOUrcE:RESidual:FREQuency:DETector:COUPled is set to ON (the default). When this is true, the following equation shows the relationship between the Carrier and Residual frequency and the Multiplier and Divisor:

$$\text{Carrier} = \text{Residual} * (\text{Multiplier} / \text{Divisor})$$

Thus, for a given Carrier frequency, the Residual source is automatically set as follows:

$$\text{Residual} = \text{Carrier} / (\text{Multiplier} / \text{Divisor})$$

## **SOURce:RESidual:POWer [:LEVel | AMPLitude]**

Specify the residual source power.

### **Command syntax**

```
SOURce:RESidual:POWer [:LEVel] [:AMPLitude] <number> [dBm]  
<number> ::= a real number (NRF data)
```

### **Example**

```
SOURce:RESidual:POWer 0
```

### **Query syntax**

```
SOURce:RESidual:POWer?
```

### **Return format**

Integer 0=OFF 1=ON

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: +10 dBm

SCPI Compliance: Instrument Specific.

## 16 **STATus Commands**


- [STATus Commands Introduction](#) 280
- [STATus:ADVise:ENABLE](#) 283
- [STATus:OPERation:CONDITION?](#) 284
- [STATus:OPERation:ENABLE](#) 285
- [STATus:OPERation:EVENT?](#) 286
- [STATus:OPERation:NTRansition](#) 287
- [STATus:OPERation:PTRansition](#) 288
- [STATus:PRESet](#) 289
- [STATus:QUEStionable:CONDITION?](#) 290
- [STATus:QUEStionable:ENABLE](#) 291
- [STATus:QUEStionable:\[EVENT\]?](#) 292
- [STATus:QUEStionable:NTRansition](#) 293
- [STATus:QUEStionable:PTRansition](#) 294



## **STATus Commands Introduction**


- STATus:ADVise:ENABLE (0 | OFF | 1 | ON)
- STATus:OPERation:CONDITION?
- STATus:OPERation:ENABLE (value)
- STATus:OPERation:EVENt?
- STATus:OPERation:NTRansition (value)
- STATus:OPERation:PTRansition (value)
- STATus:PRESet
- STATus:QUEStionable:CONDition?
- STATus:QUEStionable:ENABLE (value)
- STATus:QUEStionable:EVENt?
- STATus:QUEStionable:NTRansition (value)
- STATus:QUEStionable:PTRansition (value)

Also see \*ESR? \*ESE \*STB? \*SRE commands.

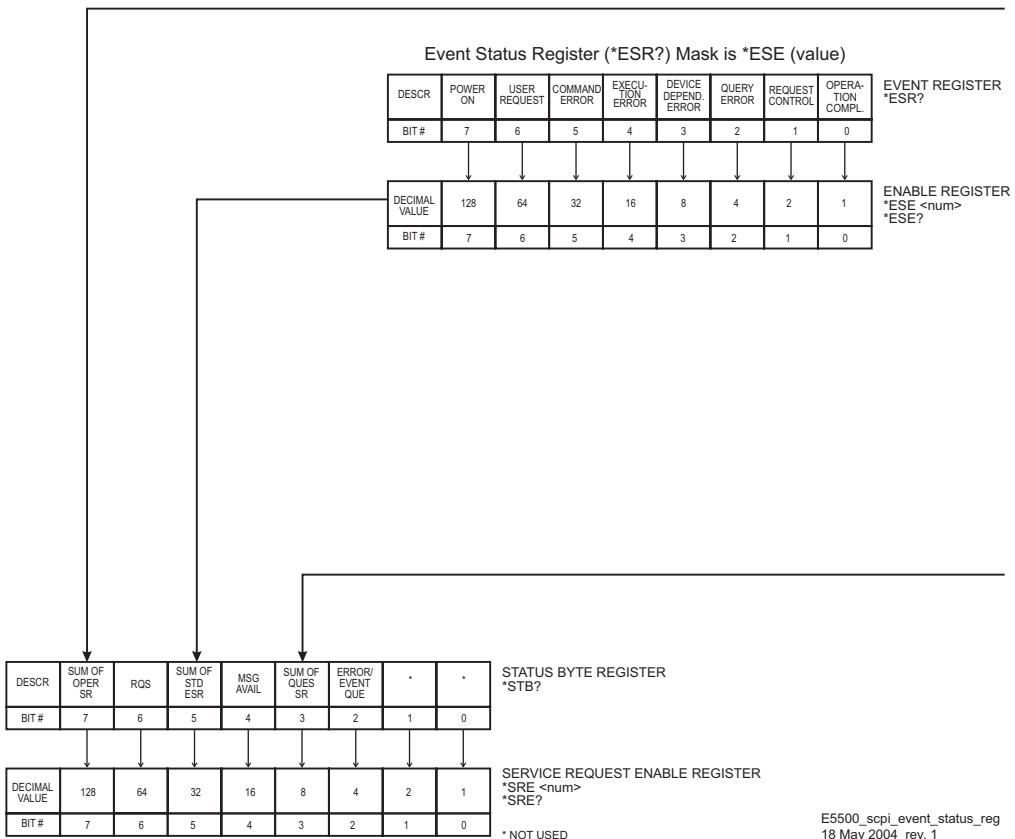

**Figure 17** Event status register 1

## 16 STATus Commands

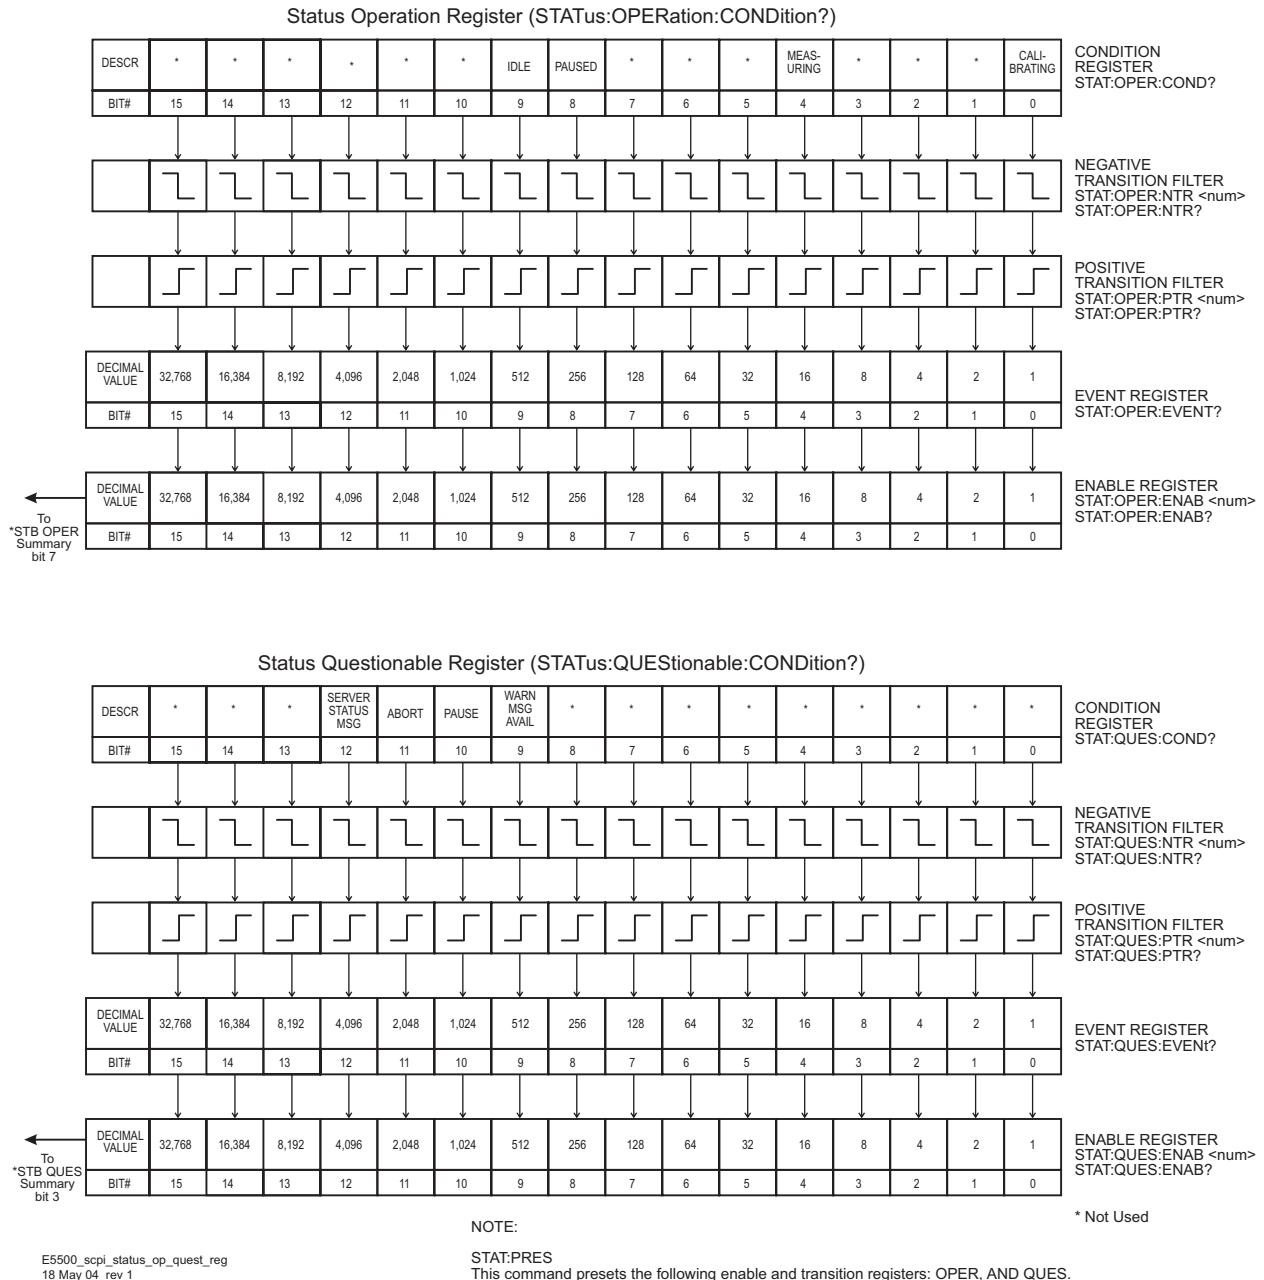

**Figure 18** Event status register 2

## STATus:ADVise:ENABLE

When set to ON, server status messages (non-error) are also placed in the SCPI error queue and bit 12 of the Questionable Status Register is activated to report when messages are available.

### Command syntax

```
STATus:ADVise:ENABLE OFF|0|ON|1
```

### Example

```
STATus:ADVise:ENABLE ON
```

### Query syntax

```
STATus:ADVise:ENABLE?
```

### Return format

Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: OFF

SCPI Compliance: Standard

## **STATus:OPERation:CONDITION?**

Provides information about the state of the measurement system. Condition registers continually monitor the state of the system. There is no buffering for this register, its status is updated in real time.

### **Command syntax**

Query Only

### **Query syntax**

STATus:Operation:CONDITION?

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

- bit 0 = 1 = Calibrating
- bit 4 = 16 = Measuring
- bit 8 = 256 = Paused
- bit 9 = 512 = Idle
- All other bits are not used.

Reading the Condition register is nondestructive.

## STATus:OPERation:ENABLE

Specifies which bits in the STATus:OPERation:EVENt register set the Operation Register Summary Bit (bit 7) in the Status Byte (\*STB?).

### Command syntax

```
STATus:OPERation:ENABLE <num>
```

### Example

```
STATus:OPERation:ENABLE
```

### Query syntax

```
STATus:OPERation:ENABLE?
```

### Return format

Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Standard

### Additional information

STATus:PREset clears this enable register.

## **STATus:OPERation:EVENT?**

EVENt registers latch events from the CONDITION register as specified by the PTRansition and NTRansition registers.

### **Command syntax**

Query Only

### **Query syntax**

STATus:OPERation:EVENT?

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

- STATus: QUEstionable:EVENT? Clears the event register (destructive read).
- \*CLS clears the event register.

## STATus:OPERation:NTRansition

Transition filters specify what type of bit state transition in the :CONDITION register will set corresponding bits in the :EVENT register. Transition filter bits may be set for positive transitions :PTRansition (0 to 1), negative transitions :NTRansition (1 to 0) or both.

### Command syntax

```
STATus:OPERation:NTRansition
```

### Example

```
STATus:OPERation:NTRansition
```

### Query syntax

```
STATus:OPERation:NTRansition?
```

### Return format

Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### Additional information

- STATus:PREset sets all PTRansition bits to 1 and NTRansition bits to 0
- \*CLS does not affect transition registers

## **STATus:OPERation:PTRansition**

Transition filters specify what type of bit state transition in the :CONDition register will set corresponding bits in the :EVENT register. Transition filter bits may be set for positive transitions :PTRansition (0 to 1), negative transitions :NTRansition (1 to 0) or both.

### **Command syntax**

```
STATus:OPERation:PTRansition
```

### **Example**

```
STATus:OPERation:PTRansition
```

### **Query syntax**

```
STATus:OPERation:PTRansition?
```

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

- STATus:PREset sets all PTRansition bits to 1 and NTRansition bits to 0
- \*CLS does not affect transition registers

## STATus:PRESet

Presets all SCPI Status :ENABLE, :PTRANSition and :NTRANSition registers.

### Command syntax

STATus : PRESet

### Query syntax

Command Only

### Example

STATus:PRESet

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### Additional information

- :ENABLE registers bits are set to 0.
- :PTRANSition register bits are set to 1.
- :NTRANSition register bits are set to 0.
- Other registers are not affected. See \*CLS for clearing other registers.

## **STATus:QUESTIONable:CONDITION?**

Provides information about measurement warnings or errors. Condition registers continually monitor the state of the system. There is no buffering for this register, its status is updated in real time.

### **Command syntax**

Query Only

### **Query syntax**

```
STATus:QUESTIONable:CONDITION?
```

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

- bit 9 = 512 = Warning message available.
- bit 10 = 1024 = Pause      "      "
- bit 11 = 2048 = Abort      "      "
- bit 12 = 4096 = Server Status message available.
- All other bits are not used.

Reading the Condition register is nondestructive.

## STATus:QUESTIONable:ENABLE

Specifies which bits in the STATus: QUESTIONable:EVENT register set the Questionable Register Summary Bit (bit 3) in the Status Byte (\*STB?).

### Command syntax

```
STATus :QUESTIONable:ENABLE
```

### Example

```
STATus :QUESTIONable:ENABLE 3584
```

### Query syntax

```
STATus :QUESTIONable:ENABLE?
```

### Return format

Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: 0

SCPI Compliance: Standard

### Additional information

STATus:PREset clears this enable register.

## **STATus:QUEStionable:[EVENT]?**

EVENt registers latch events from the CONDITION register as specified by the PTRansition and NTRansition registers.

### **Command syntax**

Query Only

### **Query syntax**

STATus:QUEStionable: [EVENT] ?

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

- STATus: QUEStionable:EVENt? Clears the event register (destructive read).
- \*CLS clears the event register.

## STATus:QUESTIONable:NTRansition

Transition filters specify what type of bit state transition in the :CONDITION register will set corresponding bits in the :EVENT register. Transition filter bits may be set for positive transitions :PTRansition (0 to 1), negative transitions :NTRansition (1 to 0) or both.

### Command syntax

```
STATus:QUESTIONable:NTRansition
```

### Example

```
STATus:QUESTIONable:NTRansition 2560
```

### Query syntax

```
STATus:QUESTIONable:NTRansition?
```

### Return format

Integer

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### Additional information

- STATus:PREset sets all PTRansition bits to 1 and NTRansition bits to 0
- \*CLS does not affect transition registers

## **STATus:QUESTIONable:PTRansition**

Transition filters specify what type of bit state transition in the :CONDITION register will set corresponding bits in the :EVENT register. Transition filter bits may be set for positive transitions :PTRansition (0 to 1), negative transitions :NTRansition (1 to 0) or both.

### **Command syntax**

```
STATus:QUESTIONable:PTRansition
```

### **Example**

```
STATus:QUESTIONable:PTRansition 2560
```

### **Query syntax**

```
STATus:QUESTIONable:PTRansition?
```

### **Return format**

Integer

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

- STATus:PREset sets all PTRansition bits to 1 and NTRansition bits to 0
- \*CLS does not affect transition registers

## 17 **SYSTem Commands**

- SYSTem Commands Introduction 296
- SYSTem:ASSet:CALSource 297
- SYSTem:ASSet:CARRier 298
- SYSTem:ASSet:COUNter 299
- SYSTem:ASSet:DCONverter 300
- SYSTem:ASSet:DCONverter:USAGE 301
- SYSTem:ASSet:FFT 302
- SYSTem:ASSet:FFT:CUSTom[:SEGTable] 303
- SYSTem:ASSet:PSHifter 304
- SYSTem:ASSet:REFerence 305
- SYSTem:ASSet:RESidual 306
- SYSTem:ASSet:SLAVe:SOURce 307
- SYSTem:ASSet:SLAVe:SOURce:PORT 308
- SYSTem:ASSet:SWANalyzer 309
- SYSTem:ASSet:SWANalyzer:CUSTom [:SEGTable] 310
- SYSTem:ASSet:TBASe 311
- SYSTem:ASSet:TSET 312
- SYSTem:ERRor? 313
- SYSTem:GUI:LLOCKout[:STATe] 316
- SYSTem:GUI:REMote[:STATe] 317
- SYSTem:HELP:HEADers? 318
- SYSTem:PATH:CARRier 319
- SYSTem:PATH:DCBAnalyzer 320
- SYSTem:PATH:FFTAnalyzer 321
- SYSTem:PATH:SWANalyzer 322
- SYSTem:PATH:TVCO 323
- SYSTem:TStart? 324
- SYSTem:VERSion? 325



## SYSTem Commands Introduction

Use the SYSTem commands to select system assets and perform miscellaneous system functions.

The commands in this subsystem have the following command hierarchy:

- SYSTem:ASSet:CALSource ("None" | "asset\_name")
- SYSTem:ASSet:CARRier ("None" | "asset\_name")
- SYSTem:ASSet:COUNter ("None" | "asset\_name")
- SYSTem:ASSet:DCONverter ("None" | "asset\_name")
- SYSTem:ASSet:DCONverter:USAGe (NONE | MANual | SYSTem)
- SYSTem:ASSet:FFT ("None" | "asset\_name")
- SYSTem:ASSet:FFT:CUSTom:[SEGTable]
- SYSTem:ASSet:PSHifter ("None" | "asset\_name")
- SYSTem:ASSet:REFERENCE ("None" | "asset\_name")
- SYSTem:ASSet:RESidual ("None" | "asset\_name")
- SYSTem:ASSet:SLAVe:SOURce ("None" | "asset\_name")
- SYSTem:ASSet:SLAVe:SOURce:PORT (LOINput | AUXinput)
- SYSTem:ASSet:SWANalyzer (value)
- SYSTem:ASSet:SWANalyzer:CUSTom:[SEGTable]
- SYSTem:ASSet:TBASe ("None" | "asset\_name")
- SYSTem:ASSet:TSET ("None" | "asset\_name")
- SYSTem:ERRor?
- SYSTem:GUI:LLOCKout[:STATe]
- SYSTem:GUI:REMote[:STATe] (0 | OFF | 1 | ON)
- SYSTem:HELP:HEADers?
- SYSTem:PATH:CARRier (TSET | DCONverter)
- SYSTem:PATH:DCBBanalyzer (TSLF | TSHF | TSRF)
- SYSTem:PATH:FFTAalyzer (TSLF | TSHF | TSRF | DCRF)
- SYSTem:PATH:SWANalyzer (TSLF | TSHF | TSRF | DCRF)
- SYSTem:PATH:TVCO (FPANel | RPANel | INTernal)
- SYSTem:TStArt?
- SYSTem:VERSion?

## SYSTem:ASSet:CALSource

Specify the calibration source.

### Command syntax

```
SYSTem:ASSet:CALSource <"None" | "asset_name">
```

Asset\_name = quoted string as defined in the Asset Manager

### Example

```
SYSTem:ASSet: CALSource"XXXXX"  
SYSTem:ASSet: CALSource "NONE"
```

### Query syntax

```
SYSTem:ASSet: CALSource?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### Additional information

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## **SYSTem:ASSet:CARRier**

Specify the carrier source.

### **Command syntax**

SYSTem:ASSet:CARRier <“None”|”asset\_name”>

Asset\_name = quoted string as defined in the Asset Manager

### **Example**

```
SYSTem:ASSet:CARRier "XXXX"  
SYSTem:ASSet:CARRier "NONE"
```

### **Query syntax**

SYSTem:ASSet:CARRier?

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### **Additional information**

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## SYSTem:ASSet:COUNTer

Specify the counter.

### Command syntax

```
SYSTem:ASSet:CARRier <"None" | "asset_name">
```

Asset\_name = quoted string as defined in the Asset Manager

### Example

```
SYSTem:ASSet:COUNTER AUTO,"XXXXXXA-001,GPIB,11,SN12345"  
SYSTem:ASSet:COUNTER NONE
```

### Query syntax

```
SYSTem:ASSet:COUNTER?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: VFRMS (NULL)

SCPI Compliance: Instrument Specific.

### Additional information

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## **SYSTem:ASSet:DConverter**

Specify the downconverter.

### **Command syntax**

```
SYSTem:ASSet:DConverter <"None" | "asset_name">
```

Asset\_name = quoted string as defined in the Asset Manager

### **Example**

```
SYSTem:ASSet:DConverter  
AUTO,"XXXXXA-001,GPIB,11,SN12345"
```

### **Query syntax**

```
SYSTem:ASSet:DConverter?
```

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### **Additional information**

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## SYSTem:ASSet:DCONverter:USAGe

Specify if and how the down converter is to be used in the current measurement.

### Command syntax

```
SYSTem:ASSet:DCONverter:USAGe NONE|MANual|SYSTem
```

### Example

```
SYSTem:ASSet:DCONverter:USAGe SYSTem
```

### Query syntax

```
SYSTem:ASSet:DCONverter:USAGe?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NONE

SCPI Compliance: Instrument Specific.

### Additional information

If NONE is selected, the down converter is not used in the measurement. If MANual is selected, the downconverter is used in the measurement with its current settings; no commands to set the input frequency, IF gain, etc. are sent. If SYSTem is selected, the downconverter is set up through the settings on the downconverter parameters page and used in the measurement.

## **SYSTem:ASSet:FFT**

Specify the FFT analyzer.

### **Command syntax**

```
SYSTem:ASSet:FFT <"None" | "asset_name">
```

Asset\_name = quoted string as defined in the Asset Manager

### **Example**

```
SYSTem:ASSet:FFT AUTO, "XXXXX"  
SYSTem:ASSet:FFT NONE
```

### **Query syntax**

```
SYSTem:ASSet:FFT?
```

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### **Additional information**

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## SYSTem:ASSet:FFT:CUSTom[:SEGTable]

Specify the custom segment table for the FFT analyzer.

### Command syntax

```
SYSTem:ASSet:FFT:CUSTom[:SEGTable] <"path\file_name.fst">
<path\file name.fst> ::= quoted string (full or relative path and
filename) <file>
```

### Example

```
SYSTem:ASSet:FFT:CUSTom "Segtbl_1.fst"
```

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### Additional information

[:SENSe]:RANGE:FFT:SEGTable[:MEASurement][:QUALity] CUSTom must be selected to use the currently loaded custom segment table.

Custom segment tables are edited and saved using the Measurement Client GUI Define menu. The default file extension is (.fst) for Fft Segment Table.

## **SYSTem:ASSet:PSHifter**

Specify the phase shifter.

### **Command syntax**

```
SYSTem:ASSet:PSHifter <"None" | "asset_name">
```

Asset\_name = quoted string as defined in the Asset Manager

### **Query syntax**

```
SYSTem:ASSet:PSHifter?
```

### **Example**

```
SYSTem:ASSet:PSHifter "XXXXX"  
SYSTem:ASSet:PSHifter "NONE"
```

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### **Additional information**

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## SYSTem:ASSet:REFerence

Specify the reference source.

### Command syntax

```
SYSTem:ASSet:REFerence <"None" | "asset_name">
```

Asset\_name = quoted string as defined in the Asset Manager

### Example

```
SYSTem:ASSet:REFerence AUTO,"XXXXX"  
SYSTem:ASSet:REFerence "NONE"
```

### Query syntax

```
SYSTem:ASSet:REFerence?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### Additional information

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## **SYSTem:ASSet:RESidual**

Specify the residual source.

### **Command syntax**

```
SYSTem:ASSet:RESidual <"None" | "asset_name">
```

Asset\_name = quoted string as defined in the Asset Manager

### **Query syntax**

```
SYSTem:ASSet: RESidual?
```

### **Example**

```
SYSTem:ASSet: RESidual"83650A"  
SYSTem:ASSet: RESidual "NONE"
```

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### **Additional information**

Invalid asset names will be accepted, but will cause a server error message when a measurement is initialized.

## SYSTem:ASSet:SLAVe:SOURce

Specify the slave source associated with the 50kHz-1600MHz RF Output of the carrier noise test set (N5507A H16/H17). This slave source is connected to the Auxiliary Input or LO input of the carrier noise test set (see SYSTem:ASSet:SLAVe:SOURce:PORT).

### Command syntax

```
SYSTem:ASSet:SLAVe:SOURce <"None" | "asset_name">
asset_name = quoted string as defined in the Asset Manager
```

### Example

```
SYSTem:ASSet:SLAVe:SOURce "XXXXX"
SYSTem:ASSet:SLAVe:SOURce "NONE"
```

### Query syntax

```
SYSTem:ASSet:SLAVe:SOURce?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### Additional information

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

The carrier noise test set can be used as a source, with the source output port being the 50kHz-1600MHz RF Output. However, another source has to provide a signal to the carrier noise test set's divider chain.

## **SYSTem:ASSet:SLAVe:SOURce:PORT**

Specify the input port on the carrier noise test set to which the slave source is connected.

### **Command syntax**

```
SYSTem:ASSet:SLAVe:SOURce:PORT LOINput|AUXinput
```

### **Example**

```
SYSTem:ASSet:SLAVe:SOURce:PORT AUXinput
```

### **Query syntax**

```
SYSTem:ASSet:SLAVe:SOURce:PORT?
```

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: LOINput

SCPI Compliance: Instrument Specific.

### **Additional information**

- LOINput specifies the LO IN 3-6.6 GHz port
- AUXinput specifies the AUX INPUT 640-1280 MHz port.

## SYSTem:ASSet:SWANalyzer

Specify the swept analyzer.

### Command syntax

```
SYSTem:ASSet:SWANalyzer <"None" | "asset_name">  
asset_name = quoted string as defined in the Asset Manager
```

### Example

```
SYSTem:ASSet:SWANalyzer AUTO,"XXXXX"  
SYSTem:ASSet:SWANalyzer NONE
```

### Query syntax

```
SYSTem:ASSet:SWANalyzer?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### Additional information

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## **SYSTem:ASSet:SWANalyzer:CUSTom[:SEGTable]**

Specify the custom segment table to be used by the swept analyzer.

### **Command syntax**

```
SYSTem:ASSet:SWANalyzer:CUSTom[:SEGTable] <"path\filename.sst">
<"path\filename.sst"> ::= string (full or relative path and filename)
```

### **Example**

```
SYSTem:ASSet:SWANalyzer:CUSTom "Segtbl_2.sst"
```

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### **Additional information**

[:SENSe]:RANGE:SWEPt:SEGTable[:MEASurement][ :QUALity] CUSTom must be selected to use the currently loaded custom segment table.

Custom segment tables are edited and saved using the Measurement Client GUI Define menu. The default file extension is (.sst) for Swept Segment Table.

## SYSTem:ASSet:TBASe

Specify the time base.

### Command syntax

```
SYSTem:ASSet:TBASe <"None" | "asset_name">
asset_name = quoted string as defined in the Asset Manager
```

### Example

```
SYSTem:ASSet:TBASe AUTO "XXXXXX"
SYSTem:ASSet:TBASe NONE
```

### Query syntax

```
SYSTem:ASSet:TBASe?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### Additional information

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## **SYSTem:ASSet:TSET**

Specify the testset.

### **Command syntax**

SYSTem:ASSet:TSET <"None" | "asset\_name">

Asset\_name = quoted string as defined in the Asset Manager

### **Example**

```
SYSTem:ASSet:TSET "N5500A"  
SYSTem:ASSet:TSET "NONE"
```

### **Query syntax**

SYSTem:ASSet:TSET?

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NULL

SCPI Compliance: Instrument Specific.

### **Additional information**

## SYSTem:ERRor?

Queries an error from the error queue.

### Command syntax

Query Only

### Query syntax

SYSTem:ERRor?

### Example

```
Return format
<value>, <string>
<value> is an integer from -32768 to +32767.
<string> the text of the error message.
```

The following is an example of one response:

-113,"Undefined header"

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### Additional information

The response for :ERRor is an ASCII string with two arguments separated by a comma. The first is an integer, ranging from -32768 to +32767, and the second is quoted string which describes the error in clear text.

For error information, refer to [Table 3](#) on page 314.

**Table 3** SCPI Error Messages

Error Number Range	E5500 Specific Errors Description
100 - 199	Abort - Measurement aborted. Body of message indicates the reason.
200 - 299	Pause Point - Measurement is paused waiting for user interaction. Body of message indicates reason.
300 - 499	Status - Incidental measurement progress. STATus: ADVise:ENABLE must be on to receive these messages.
500 - 599	Warning - Measurement will proceed. Body of message indicates reason.
Error Number	Description - General SCPI Errors
-100	Command error (unknown command)
-101	Invalid character
-102	Syntax error
-103	invalid separator
-104	Data type error
-105	GET not allowed
-108	Parameter not allowed
-109	Missing parameter
-112	Program mnemonic too long
-113	Undefined header
-121	Invalid character in number
-123	Numeric overflow
-124	Too many digits
-128	Numeric data not allowed
-130	Suffix error
-131	invalid suffix
-138	Suffix not allowed
-140	Character data error
-141	Invalid character data
-144	Character data too long
-148	Character data not allowed
-150	String data error

**Table 3** SCPI Error Messages (continued)

<b>Error Number Range</b>	<b>E5500 Specific Errors Description</b>
-151	Invalid string data
-158	String data not allowed
-160	Block data error
-161	invalid block data
-168	Block data not allowed
-170	Expression error
-171	Invalid Expression
-178	Expression data not allowed
-200	Execution error
-211	Trigger ignored
-221	Settings conflict
-222	Data out of range
-223	Too much data
-310	System error
-350	Too many errors
-400	Query error
-410	Query INTERRUPTED
-420	Query UNTERMINATED
-430	Query DEADLOCKED
-440	Query UNTERMINATED after indefinite response

## **SYSTem:GUI:LLOCKout[:STATe]**

Disable Measurement Development Client GUI Local menu function.

### **Command syntax**

```
SYSTem:GUI:LLOCKout
```

### **Example**

```
SYSTem:GUI:LLOCKout
```

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: unaffected

SCPI Compliance: Instrument Specific.

### **Additional information**

Invalid asset names will be accepted but will cause a server error message when a measurement is initialized.

## SYSTem:GUI:REMote[:STATe]

If ON put Measurement Development Client GUI in Remote mode. If OFF MDC GUI is in Local mode.

### Command syntax

```
SYSTem:GUI:REMote [:STATe] <boolean>
<boolean> ::= OFF | 0 | ON | 1
```

### Example

```
SYSTem:GUI:REMote ON
```

### Query syntax

```
SYSTem:GUI:REMote?
```

### Return format

Integer 0=OFF 1=ON

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: unaffected

SCPI Compliance: Instrument Specific.

### Additional information

The GUI must already be in remote or this command has no effect. Returning the GUI to Local (SYSTem:GUI:REMote OFF) cancels Local Lockout.

## **SYSTem:HELP:HEADers?**

Queries a listing of all the remote programming commands.

### **Command syntax**

Query Only

### **Query syntax**

SYSTem:HELP:HEADers?

### **Return format**

ASCII block

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Standard

### **Additional information**

The response for :HEADers is the entire SCPI tree, one ASCII line at a time.  
Each line contains a complete SCPI statement and it's query ability.

## SYSTem:PATH:CARRier

Specify the signal input port that the carrier signal is connected to.

### Command syntax

```
SYSTem:PATH:CARRier TSET|DCONverter
```

### Example

```
SYSTem:PATH:CARRier TSET
```

### Query syntax

```
SYSTem:PATH:CARRier?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: TSET

SCPI Compliance: Instrument Specific.

## **SYSTem:PATH:DCBBanalyzer**

Specify the analyzer output port that the downconverter baseband analyzer input port is connected to.

### **Command syntax**

```
SYSTem:PATH:DCBBanalyzer TSLF|TSHF|TSRF
```

### **Example**

```
SYSTem:PATH:DCBBanalyzer TSLF
```

### **Query syntax**

```
SYSTem:PATH:DCBBanalyzer?
```

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: TSRF

SCPI Compliance: Instrument Specific.

### **Additional information**

- TSLF - Test Set Low Frequency analyzer output port (Analyzer <100kHz)
- TSHF - Test Set High Frequency analyzer output port (Analyzer <100MHz)
- TSRF - Test Set RF Analyzer output port

## SYSTem:PATH:FFTAnalyzer

Specify the analyzer output port that the FFT analyzer is connected to.

### Command syntax

```
SYSTem:PATH:FFTAnalyzer TSLF|TSHF|TSRF|DCRF
```

### Example

```
SYSTem:PATH:FFTAnalyzer TSLF
```

### Query syntax

```
SYSTem:PATH:FFTAnalyzer?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: TSHF

SCPI Compliance: Instrument Specific.

### Additional information

- TSLF - Test Set Low Frequency analyzer output port (Analyzer <100kHz)
- TSHF - Test Set High Frequency analyzer output port (Analyzer <100MHz)
- TSRF - Test Set RF Analyzer output port
- DCRF - Downconverter RF Analyzer output port

## **SYSTem:PATH:SWAnalyzer**

Specify the analyzer output port that the Swept (RF) Analyzer is connected to.

### **Command syntax**

```
SYSTem:PATH:FFTAnalyzer TSLF|TSHF|TSRF|DCRF
```

### **Example**

```
SYSTem:PATH:FFTAnalyzer TSLF
```

### **Query syntax**

```
SYSTem:PATH:FFTAnalyzer?
```

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: TSRF

SCPI Compliance: Instrument Specific.

### **Additional information**

- TSLF - Test Set Low Frequency analyzer output port (Analyzer <100kHz)
- TSHF - Test Set High Frequency analyzer output port (Analyzer <100MHz)
- TSRF - Test Set RF Analyzer output port
- DCRF - Downconverter RF Analyzer output port

## SYSTem:PATH:TVCO

Specifies which port is selected to supply the tune voltage output.

### Command syntax

```
SYSTem:PATH:TVCO {FPANel|RPANel|INTernal}
```

### Example

```
SYSTem:PATH:TVCO FPANel
```

### Query syntax

```
SYSTem:PATH:TVCO?
```

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: FPANel

SCPI Compliance: Instrument Specific.

## **SYSTem:TStart?**

Query the start time of the measurement.

### **Command syntax**

Query Only

### **Query syntax**

SYSTem:TStart?

### **Return format**

String

### **Attribute summary**

Synchronization Required: none

Preset (\*RST) State: NA

SCPI Compliance: Instrument Specific.

## SYSTem:VERSion?

Queries the version of SCPI the E5500 complies with.

### Command syntax

Query Only

### Query syntax

SYSTem:VERSion?

### Return format

String

### Attribute summary

Synchronization Required: none

Preset (\*RST) State: "1995.0"

SCPI Compliance: Standard

### Additional information

The response for :VERSion is an ASCII string numeric value in <N2> format. The value returned represents the SCPI compatibility and is in the form YYYY.V. Where YYYY is the year and the V is the revision with that year.

