

Agilent Technologies N5244/45AS Option H85

User's and Service Guide

Microwave PNA-X Series High Power Configurable Test Set

PNA Series Network Analyzer On-line Help System

Application Note 1408-10



Agilent Technologies

Manufacturing Part Number: N5245-90002

Printed in USA: September 2009

Supersede August 2009

© Copyright 2009 Agilent Technologies, Inc. All rights reserved.

Warranty Statement

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED “AS IS,” AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, AGILENT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. AGILENT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD AGILENT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

DFARS/Restricted Rights Notice

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as “Commercial computer software” as defined in DFAR 252.227-7014 (June 1995), or as a “commercial item” as defined in FAR 2.101(a) or as “Restricted computer software” as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies’ standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notes

The following safety notes are used throughout this document. Familiarize yourself with each of these notes and its meaning before performing any of the procedures in this document.

WARNING	Warning denotes a hazard. It calls attention to a procedure which, if not correctly performed or adhered to, could result in injury or loss of life. Do not proceed beyond a warning note until the indicated conditions are fully understood and met.
----------------	---

CAUTION	Caution denotes a hazard. It calls attention to a procedure that, if not correctly performed or adhered to, could result in damage to or destruction of the instrument. Do not proceed beyond a caution sign until the indicated conditions are fully understood and met.
----------------	---

Definitions

- *Specifications* describe the performance of parameters covered by the product warranty (temperature –0 to 55 °C, unless otherwise noted.)
- *Typical* describes additional product performance information that is not covered by the product warranty. It is performance beyond specification that 80% of the units exhibit with a 95% confidence level over the temperature range 20 to 30 °C. Typical performance does not include measurement uncertainty.
- *Nominal* values indicate expected performance or describe product performance that is useful in the application of the product, but is not covered by the product warranty.
- *Characteristic Performance* describes performance parameter that the product is expected to meet before it leaves the factory, but is not verified in the field and is not covered by the product warranty. A characteristic includes the same guard bands as a specification.

N5244/45AS Option H85

Introduction	2
Description	2
What You Need to Know About Your N524xAS PNA-X	3
N5244/45AS Option H85 Ordering Configuration (serial tag options)	3
N5244/45A Option H85 Shipped Configuration (about network analyzer option field)	4
Operation	5
Specifications: Front Panel Jumpers and Test Ports	20
Example: Making High Power Measurements With Option H85	24
Typeface Key Conventions	24
Initial Setup	25
Determining Power Levels	26
Additional Setup	29
Selecting Power Ranges and Attenuator Settings	30
Final Setup	34
Specification	37
Service Information	37
Replaceable Parts	38
Safety and Regulatory Information	40
Introduction	40
Before Applying Power	40
Connector Care and Cleaning	40
Declaration of Conformity	40
Statement of Compliance	40
General Safety Considerations	41
Safety Earth Ground	41
Cautions applicable this instrument	41
Servicing	42
Regulatory Information	43
Instrument Markings	43
Compliance with German FTZ Emissions Requirements	44
Compliance with German Noise Requirements	44
EMC Information	44
Safety Information	44
Electrostatic Discharge Protection	45
Agilent Support and Assistance	46
Service and Support Options	46
Contacting Agilent	46
Shipping Your Analyzer to Agilent for Service or Repair	46

N5244/45AS Option H85

Introduction

This document describes the differences between the standard N5244/45A and the N5244/45AS Option H85 PNA-X Series Network Analyzer. For more technical information refer to Agilent 2-Port and 4-Port PNA-X Network Analyzer Data Sheet and Technical Specifications (N5245-90008).

Information can be viewed or printed regarding the N5244/45A PNA-X Series Network Analyzer Data sheets, white papers, or manuals by visiting our web site at <http://www.agilent.com/find/pna>, or by typing N5244A or N5245A in the search field.

Description

The Agilent N5244/45AS Option H85 is a modified version of the standard N5244/45A PNA-X Series Network Analyzer. Option H85 is designed to permit insertion of high power amplifiers, and other signal conditioning equipment, to allow high power network measurements at RF levels up to 20 watts (+43 dBm) from 10 MHz to 50 GHz. The Option H85 modification supplies extended power range attenuators *without* bias tees. The N5244/45AS Option 285 (add extended power range to 2-Port analyzer, no bias-tees) replaces the standard N5244/45A Option 219 (add extended power range and bias-tees to 2-Port analyzer). The N5244/45AS Option 485 (add extended power range to 4-Port analyzer, no bias-tee) replaces the standard N5244/45A Option 419 (add extended power range and bias-tees to 4-Port analyzer).

The Option H85 does not increase the output power of the N5244/45A analyzer. This option only allows the N5244/45A analyzer to make high power measurements. The user must supply their own amplifier(s) and external components such as high power couplers, attenuators and isolators to configure the analyzer for high power. These components are not supplied, or included with the Option H85. The user is responsible to ensure that these components meet their DUT requirements, and also protect the PNA-X from damage. Therefore, it is very important that you read this document thoroughly and follow the power level guidelines in [Table 1 on page 21](#).

NOTE The Bias Tee's are removed from the Option H85 to allow high power operation. Specifications for the Agilent N5244/45AS Option H85, when configured in Standard Configuration, are the same as those of an N5244/45A PNA-X Series Network Analyzer with Options N5244/45A-219, or N5244/45A-419.

The instrument is shipped from the factory with jumper cables installed on the front panel in what is referred to as the “Standard Configuration.” Refer to [Figure 7 on page 8](#) through [Figure 9 on page 9](#). This configuration will allow the instrument to operate as a standard N5244/45A PNA-X Series Network Analyzer with Options N5244/45A-219 or N5244/45A-419.

What You Need to Know About Your N524xAS PNA-X

Your N524xAS PNA-X network analyzer was setup as an ordering convenience to respond to customer application and test needs requiring modification or enchantment to the standard N524xA PNA-X. All AS models are tested to the performance closest matching their configuration. Test and environmental specifications, characteristics, or typical values, are based, leveraged or derived from the performance of the standard N524xA PNA-X network analyzers and their options.

Ordering configurations and rear panel serial tags will differ from the standard model number and options indicated on the network analyzer front panel, and option field window of the instrument. When ordering and enabling Option H85, Options 219/419 become Options 285/485.

N5244/45AS Option H85 Ordering Configuration (*serial tag options*)

Figure 1 Serial Tag



2-Port Configuration Includes the Following Options:


- 200 2-Ports, single source
- 285 Add extended power range to 2-Port analyzer (no bias tees)
- H85 High Power Configurable

4-Port Configuration Includes the Following Options:

- 400 4-Ports, dual source
- 485 Add extended power range to 4-Port analyzer (no bias tees)
- H85 High Power Configurable

N5244/45A Option H85 Shipped Configuration (*about network analyzer option field*)

Figure 2 About Network Analyzer

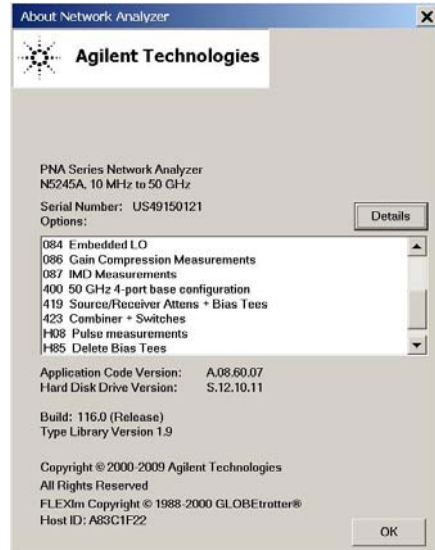

2-Port Configuration Shown in PNA-X Option Fields:

- 200 50 GHz 2-Ports base configuration¹
- 219 Source/Receiver Attens + Bias Tees
- H85 Delete Bias Tees

4-Port Configuration Shown in PNA-X Option Fields:

- 400 50 GHz 4-Ports base configuration¹
- 419 Source/Receiver Attens + Bias Tees
- H85 Delete Bias Tees

1. The frequency is dependant on the PNA-X model.

Operation

The Agilent Option H85 can be configured differently for many applications. Included in this manual are five typical configurations:

- [Figure 10, “2-Port, Two Way High Power Configuration.”](#)
- [Figure 12, “4-Port, Four Way High Power Configuration.”](#)
- [Figure 14, “2-Port, One Way High Power Configuration.”](#)
- [Figure 16, “4-Port, One Way High Power Configuration.”](#)
- [Figure 18, “2-Port Forward DUT Configuration.”](#)

NOTE The internal firmware of the PNA-X has not been modified for this option. The power levels indicated on the Agilent N5244/45AS Option H85 may differ depending on the user configuration that is chosen.

Refer to the configuration diagrams for external component connections and/or operating constraints when utilizing the high power capability of the Agilent N5244/45AS Option H85. External components are not supplied with this option.

When using the Agilent N5244/45AS Option H85 in the high power configuration (flow through R1 Loop), the analyzers R1 Input path must be set to External. In the **Trace/Chan** drop-down menu select **Channel > Hardware Setup > Path Config**. See [Figure 29 on page 32](#). In the path configuration dialog box, select **Port 1 Reference Mixer Switch > External** and press **OK** to active the R1 Input path. See [Figure 30 on page 33](#).

CAUTION The maximum attenuator power setting for the receiver attenuator is 35 dB. The PNA-X receiver step attenuators reduce the power to the A, B, C and D receivers. Power measurements to test ports 1, 2, 3 and 4 above +35 dBm will require additional attenuation. Add the appropriate amount of attenuation that will keep the coupler arm output power below the maximum receiver inputs. Refer to [Table 1 on page 21](#).

CAUTION Prior to powering-up the booster amplifier, it is highly recommended that the user verify the RF power levels seen by the various elements of the test setup. At high power levels an incorrect power level could permanently damage the instrument. Refer to [Table 1 on page 21](#).

CAUTION To reduce risk of damaging the PNA-X or your device, reduce the initial power setting to -65 dBm at the test port. The microwave PNA-X has 44 frequency bands. The firmware turns off the RF power level during band-crossings. If you are testing a high-gain device with an ALC when the PNA-X switches bands, the power shuts down and the DUT ALC attempts to increase the gain. Microseconds later the PNA-X power returns. However, in the short time frame the DUT or the VNA may be damaged. The Band Crossings are listed in [Table 3 on page 23](#).

Figure 3 N5244/45AS Option 200 and H85 2-Port RF Block Diagram

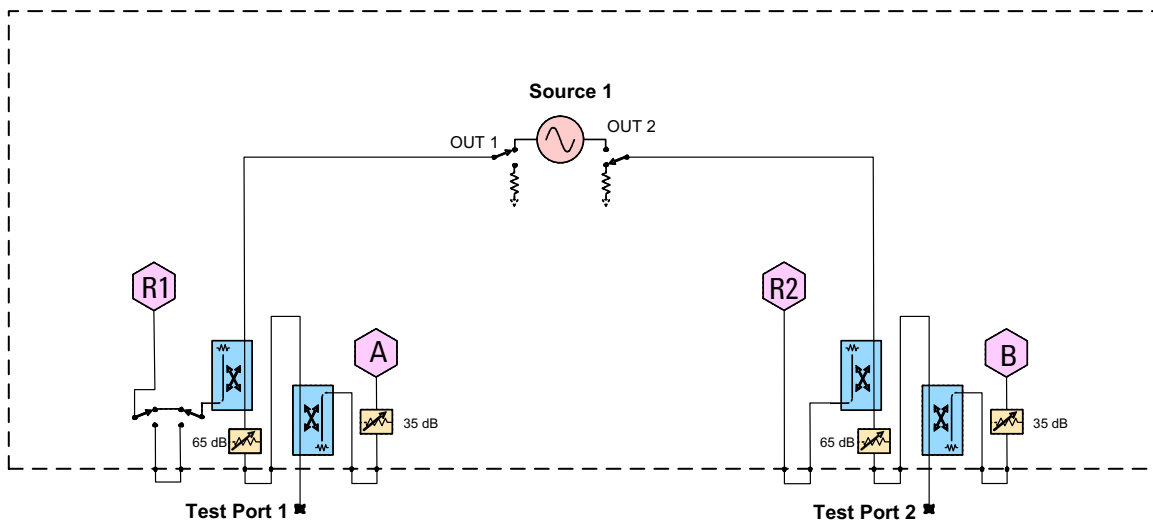


Figure 4 N5244/45AS Option 200, 224 and H85 2-Port RF Block Diagram

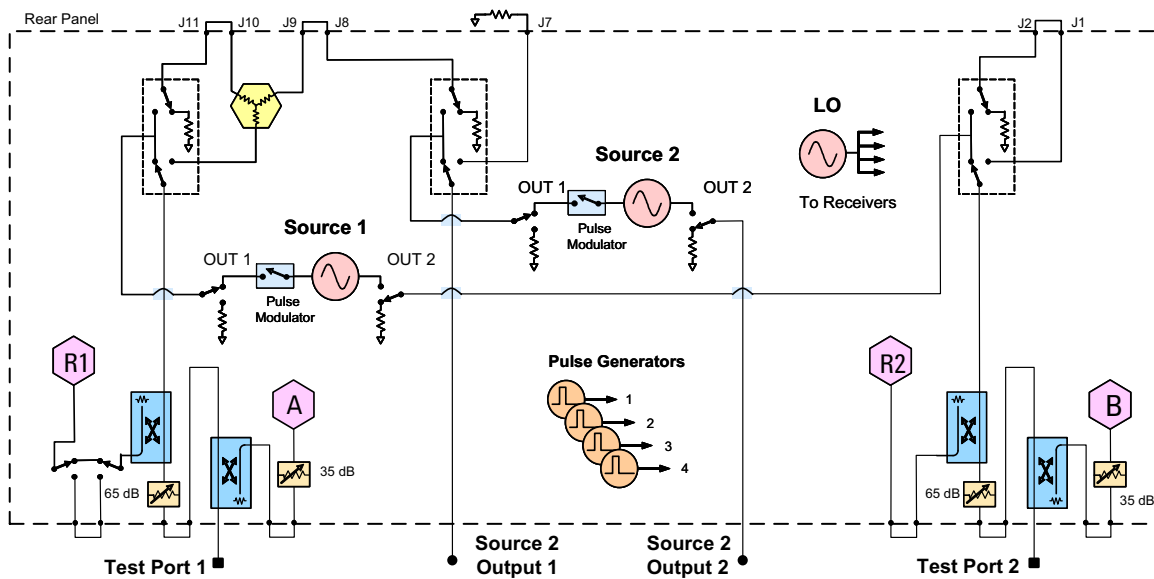


Figure 5 N5244/45AS Option 400 and H85 4-Port RF Block Diagram

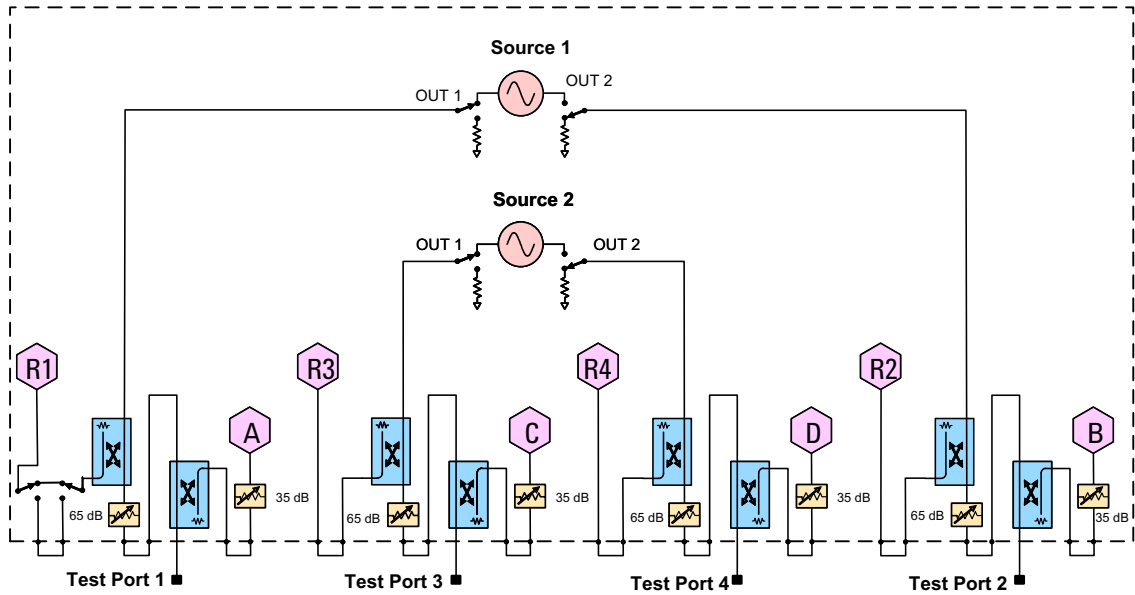


Figure 6 N5244/45AS Option 400, 423 and H85 4-Port RF Block Diagram

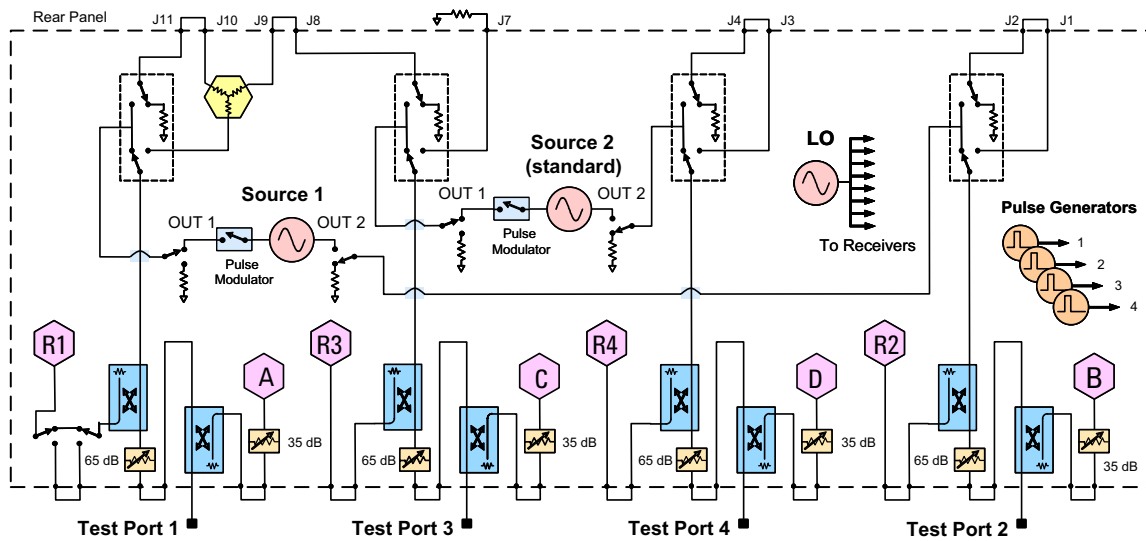


Figure 7 Standard 2-Port Front Panel

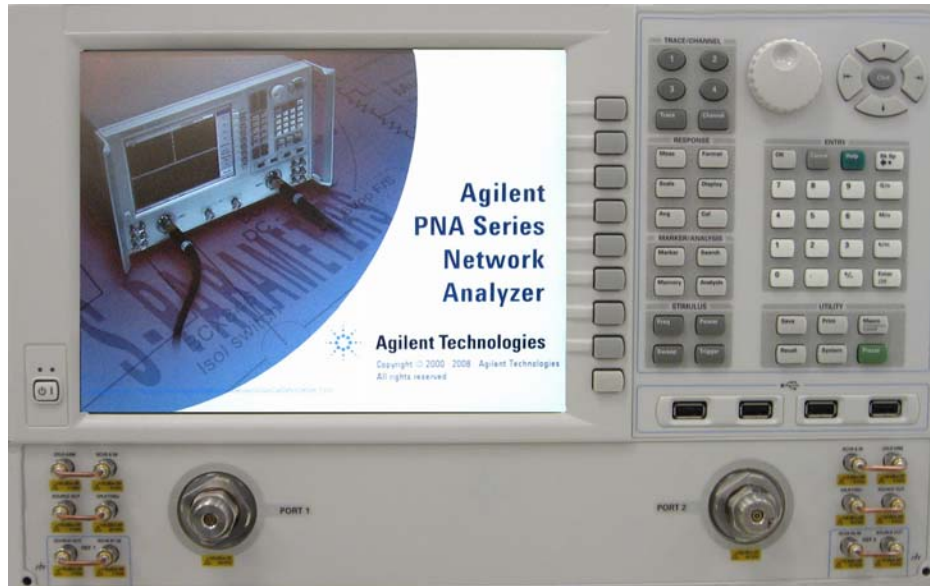


Figure 8 2-Port Front Panel with Internal Second Source


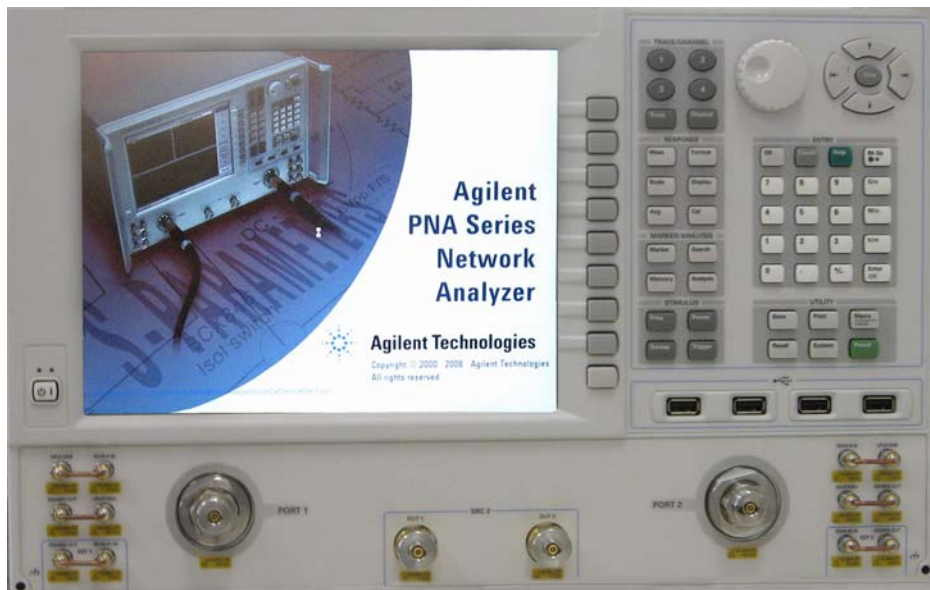


Figure 9 Standard 4-Port Front Panel

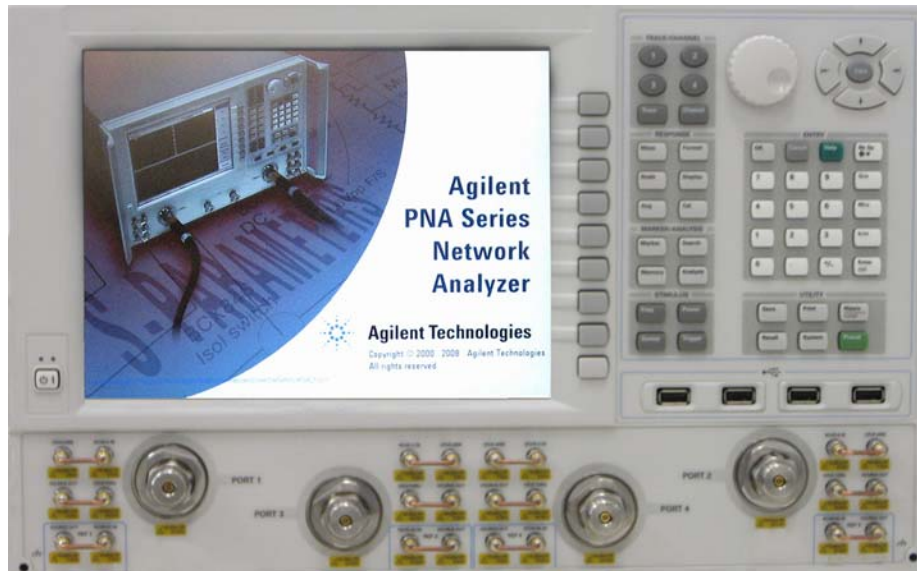

Operation

Ports 1 and 2 are configured to allow the user to stimulate each port with high power. Each port must have a high power amplifier and high power coupler. The isolators, reference and measured receiver attenuators are optional. They are dependent on the high power couplers coupling factor, amplifiers reverse isolation and power required to test the device. The attenuator, located at the high power coupler arm, may not be required if the coupling factor attenuates the signal adequately for the reference receiver channel. The same is also true for the measure receiver channels. The measure receiver attenuators for A IN and B IN may have sufficient range to compensate for the users desired power level. The isolators maybe eliminated if the amplifier reverse isolation is high. Refer to [Figure 10](#) and [Figure 11](#) on page 11.

Figure 10 2-Port, Two Way High Power Configuration


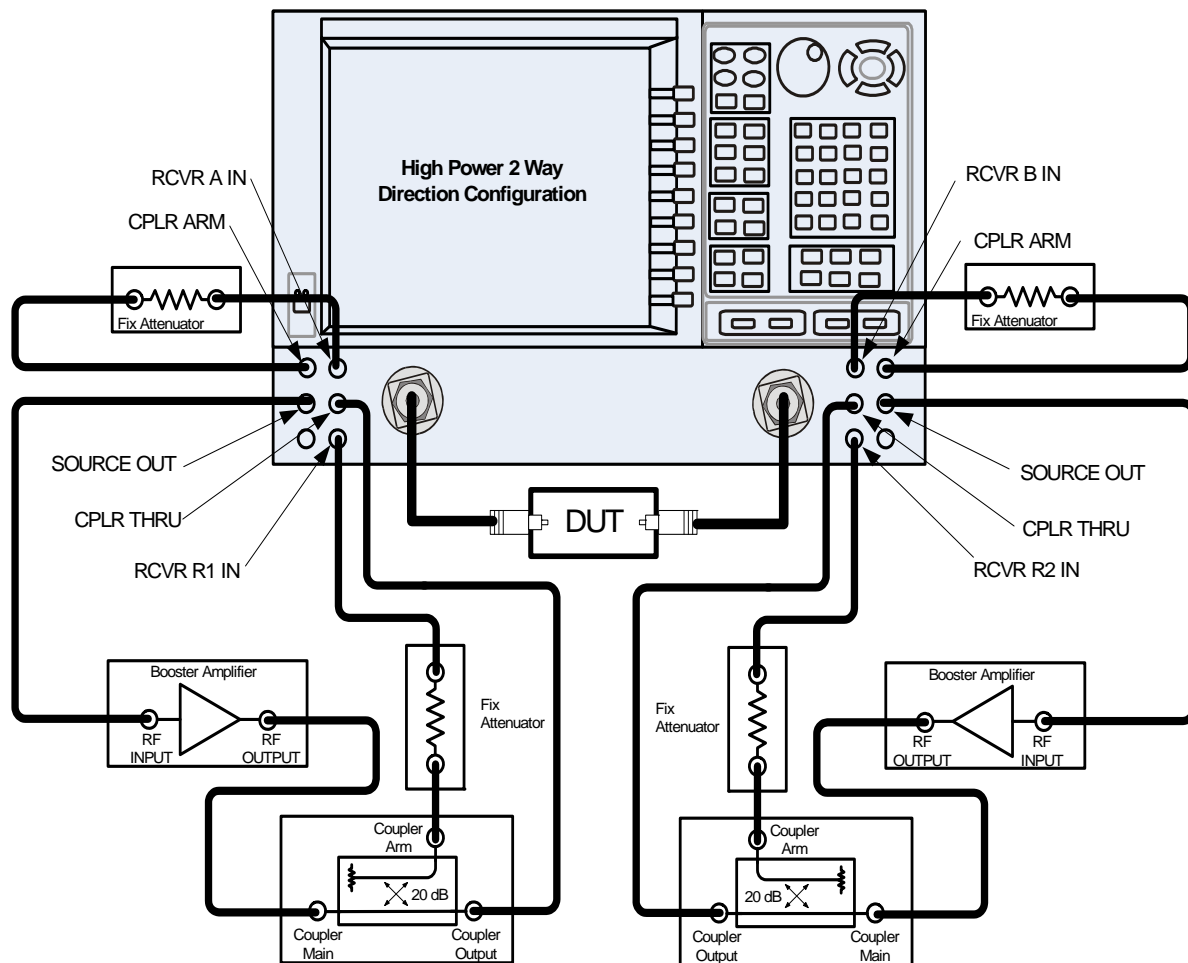


Figure 11 2-Port, Two Way High Power Block Diagram

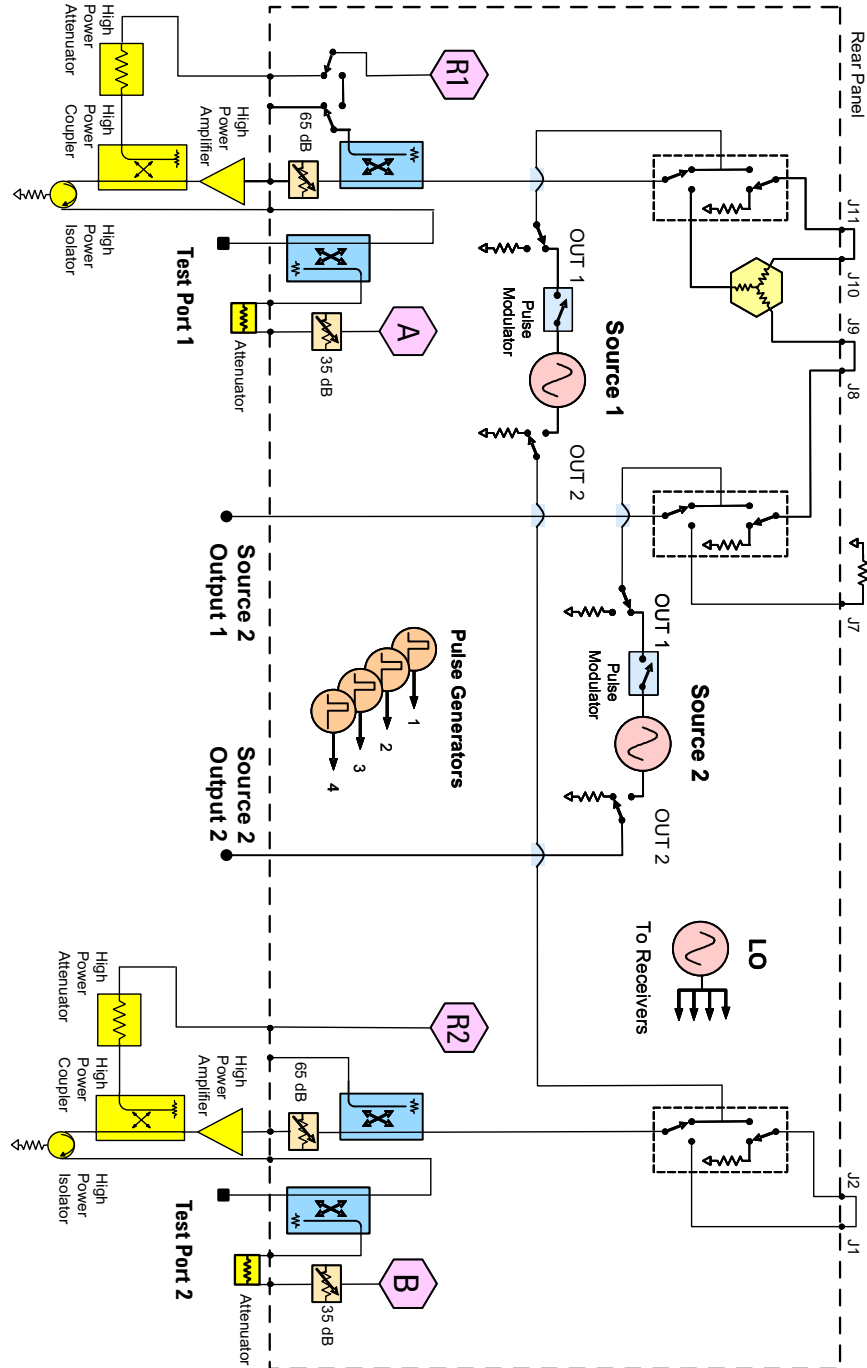

Operation

This configuration is similar to the 2-Port, Two Way Configuration with the exception of Ports 1, 2, 3 and 4 are configured to allow the user to stimulate each port with high power. Each port must have a high power amplifier, high power coupler, isolator and attenuators. The isolators, reference and measured receiver attenuators are optional. They are dependent on the high power couplers coupling factor, amplifiers reverse isolation and power required to test the device. The attenuator, located at the high power coupler arm, may not be required if the coupling factor attenuates the signal adequately for the reference receiver channel. The same is also true for the measure receiver channels. The measure receiver attenuators for A IN, B IN, C IN and D IN may have sufficient range to compensate for the users desired power level. The isolators maybe eliminated if the amplifier reverse isolation is high. The DUT is not shown in the figure. Refer to [Figure 12](#) and [Figure 13](#) on page 13.

Figure 12 4-Port, Four Way High Power Configuration


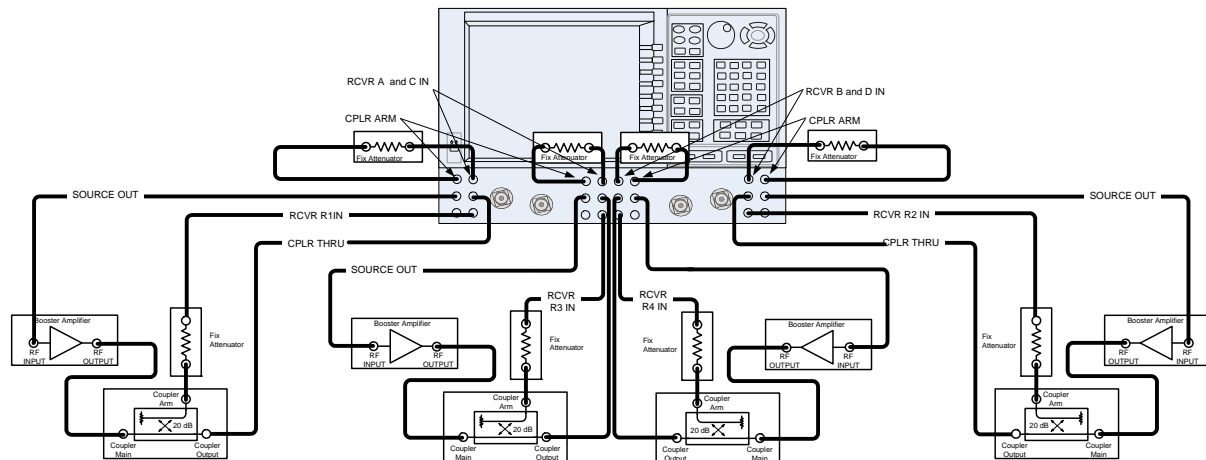


Figure 13 4-Port, Four Way High Power Block Diagram

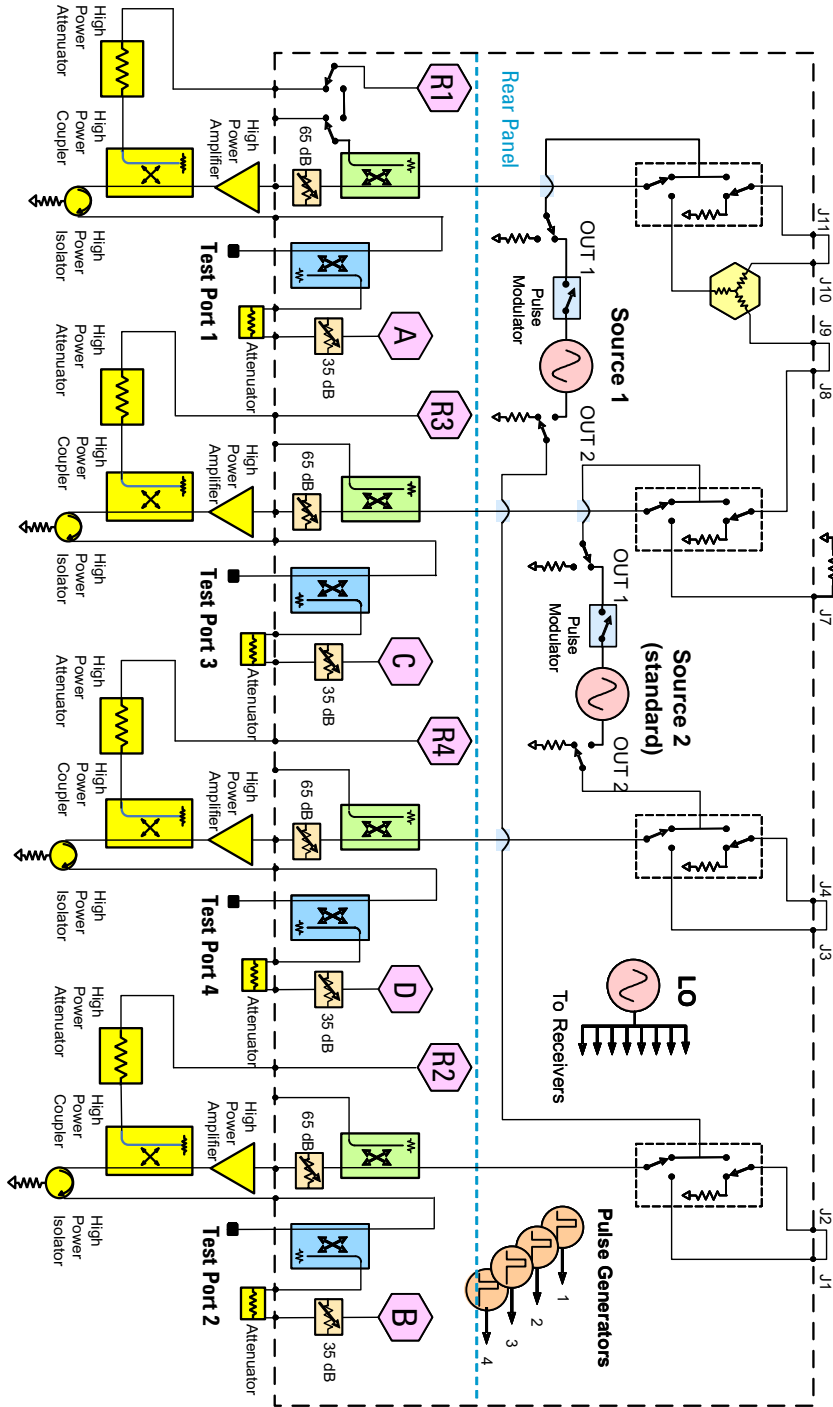

Operation

This configuration allows the user to stimulate Port 1 with high power. Port 1 must have a high power amplifier, high power coupler, isolator and attenuators. The isolator, reference and measured receiver attenuators are optional. They are dependent on the high power couplers coupling factor, amplifiers reverse isolation and power required to test the device. The attenuator, located at the high power coupler arm, may not be required if the coupling factor attenuates the signal adequately for the reference receiver channel. The same is true for the measure receiver channels. The measure receiver attenuators for A IN and B IN may have sufficient range to compensate for the users desired power level. Port 2 has a high power isolator located between the SOURCE OUT and CPLR THRU. This isolator is required to protect the components inside the PNA-X. The isolator can be replaced by a high power attenuator or circulator. Refer to [Figure 14](#) and [Figure 15](#) on page 15.

Figure 14 2-Port, One Way High Power Configuration


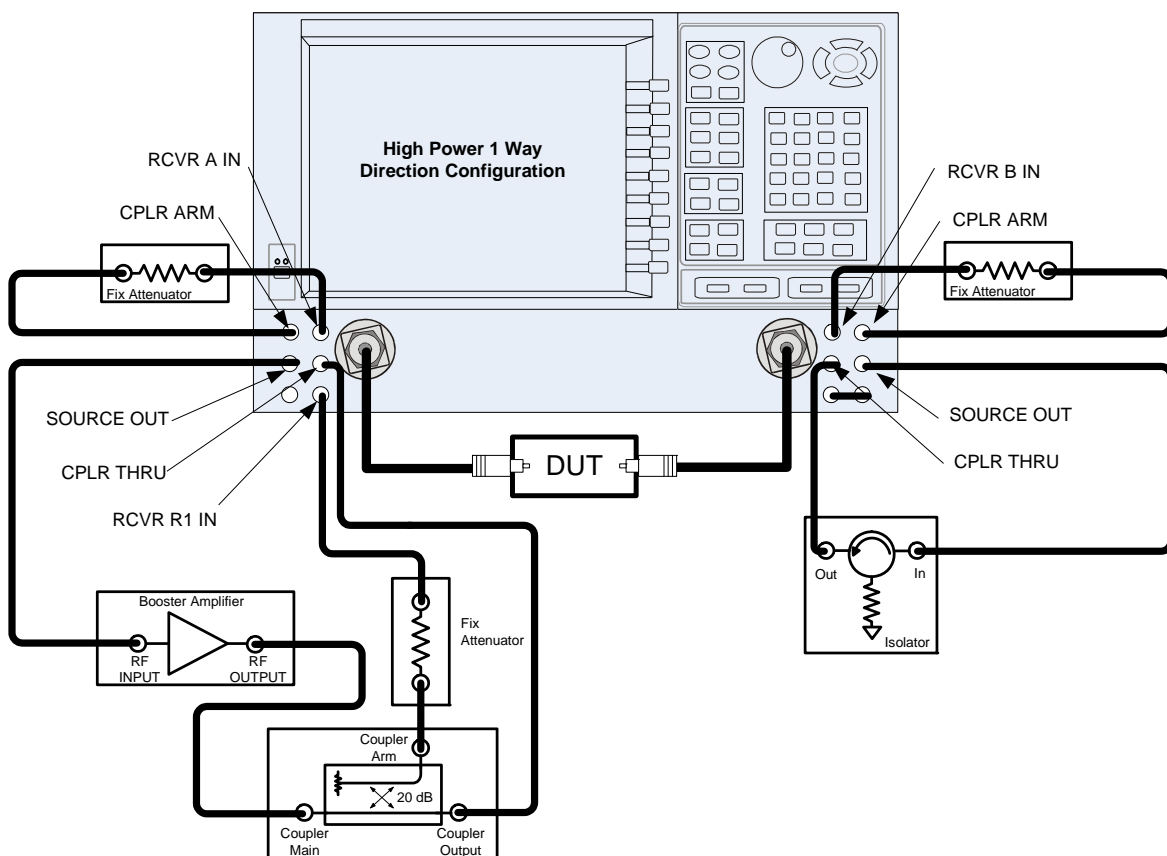


Figure 15 2-Port, One Way High Power Block Diagram

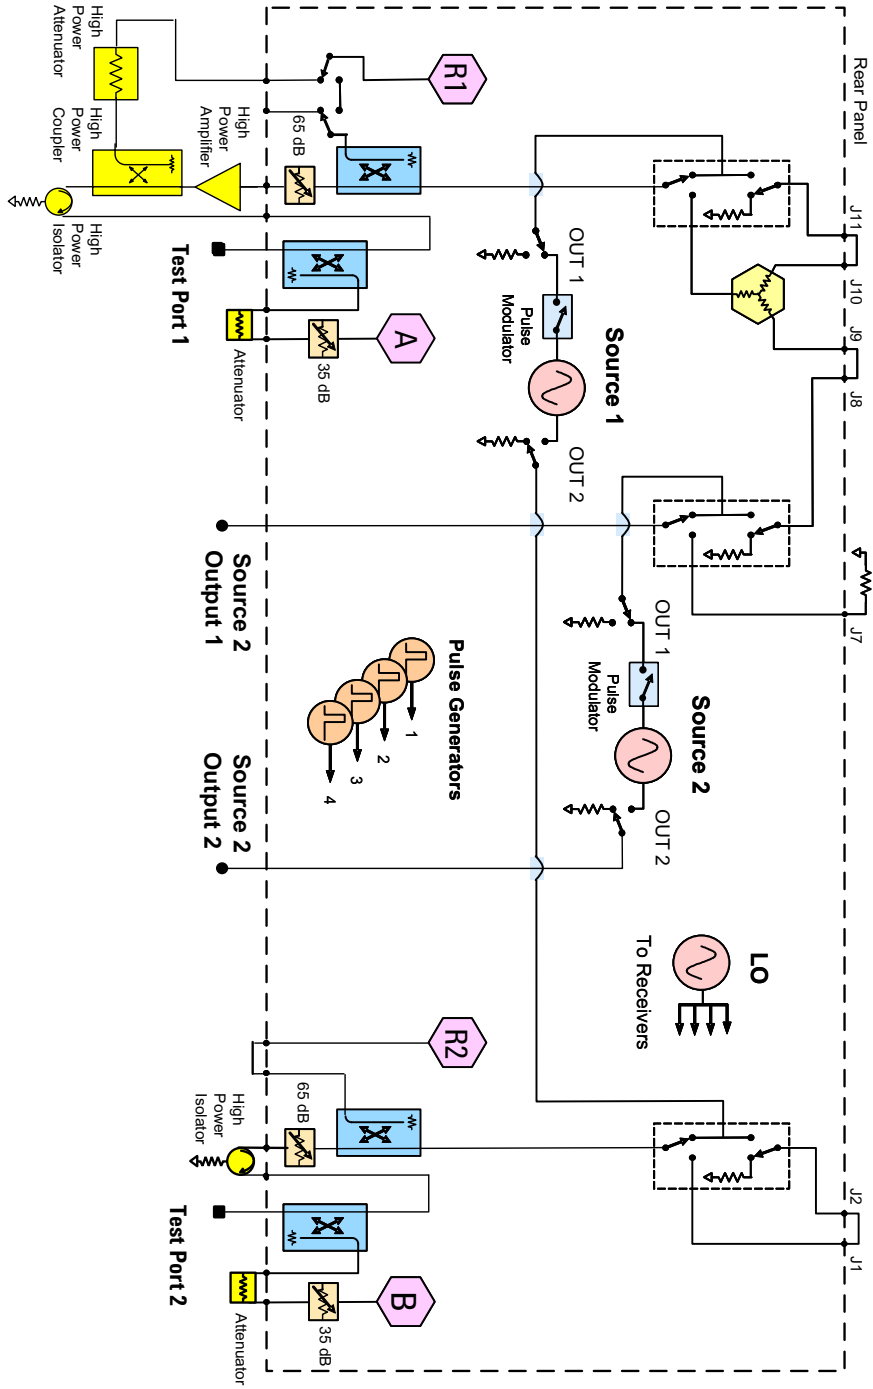

Operation

This configuration allows the user to stimulate Port 1 with high power. Port 1 must have a high power amplifier, high power coupler, isolator and attenuators. The isolator, reference and measured receiver attenuators are optional. They are dependent on the high power couplers coupling factor, amplifiers reverse isolation and power required to test the device. The attenuator, located at the high power coupler arm, may not be required if the coupling factor attenuates the signal adequately for the reference receiver channel. The same is also true for the measure receiver channels. The measure receiver attenuators for A IN, B IN, C IN and D IN may have sufficient range to compensate for the users desired power level. Ports 2, 3 and 4 each have a high power isolator located between the SOURCE OUT and CPLR THRU. This isolator is required to protect the components inside the PNA-X. The isolator can be replaced by a high power attenuator or circulator. Refer to [Figure 16](#) and [Figure 17](#) on page 17.

Figure 16 4-Port, One Way High Power Configuration


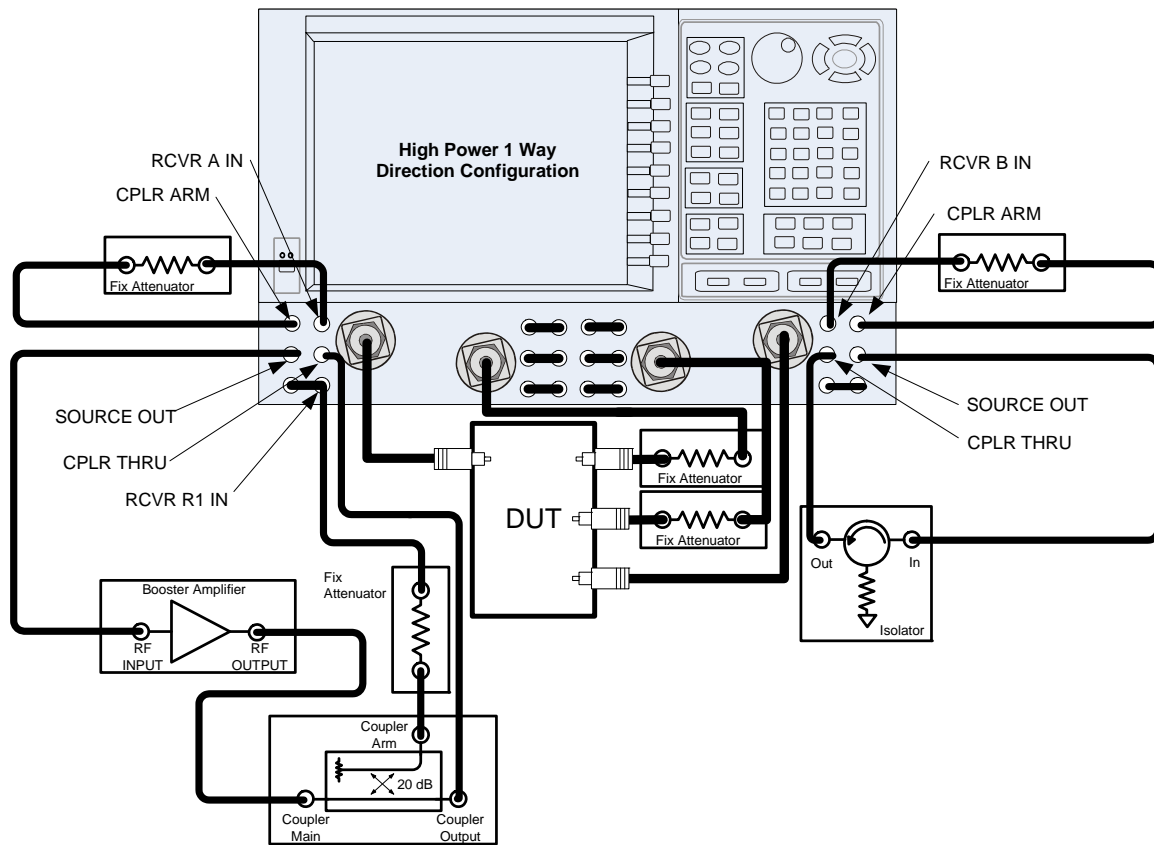


Figure 17 4-Port, One Way High Power Block Diagram

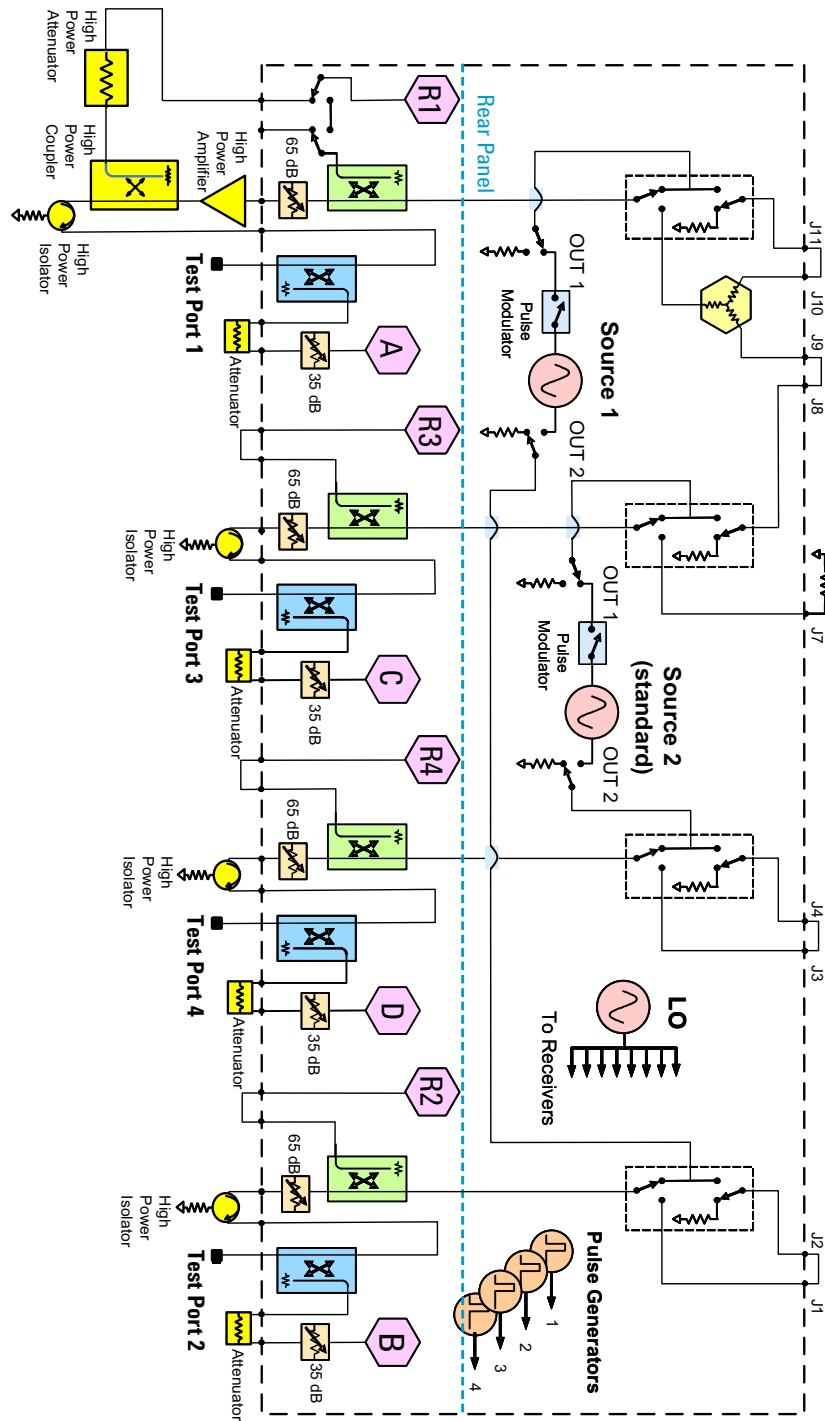

Operation

In this configuration the DUT supplies the power. The measure receiver attenuator for B IN may have sufficient range to compensate for the users desired power level. Port 2 has a high power isolator located between the SOURCE OUT and CPLR THRU. This isolator is required to protect the components inside the PNA-X. The isolator can be replaced by a high power attenuator or circulator. Reference Channel R1 can be set to internal. Refer to [Figure 18](#) and [Figure 19](#) on page 19.


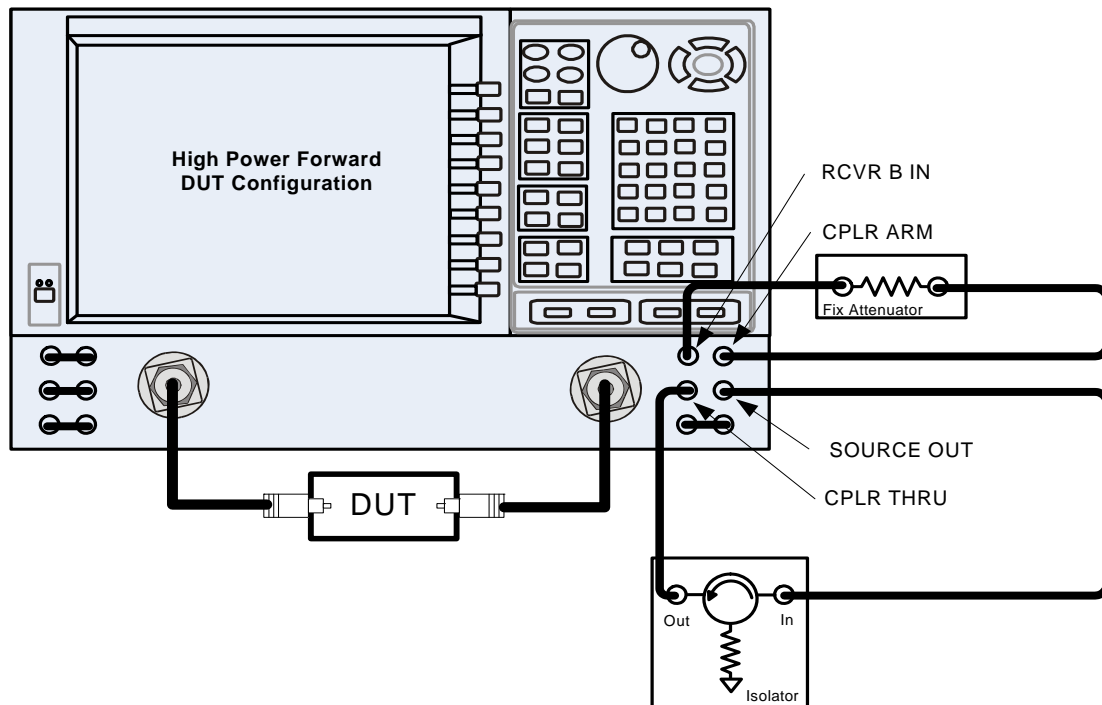
Figure 18 2-Port Forward DUT Configuration

Figure 19 2-Port Forward DUT Block Diagram

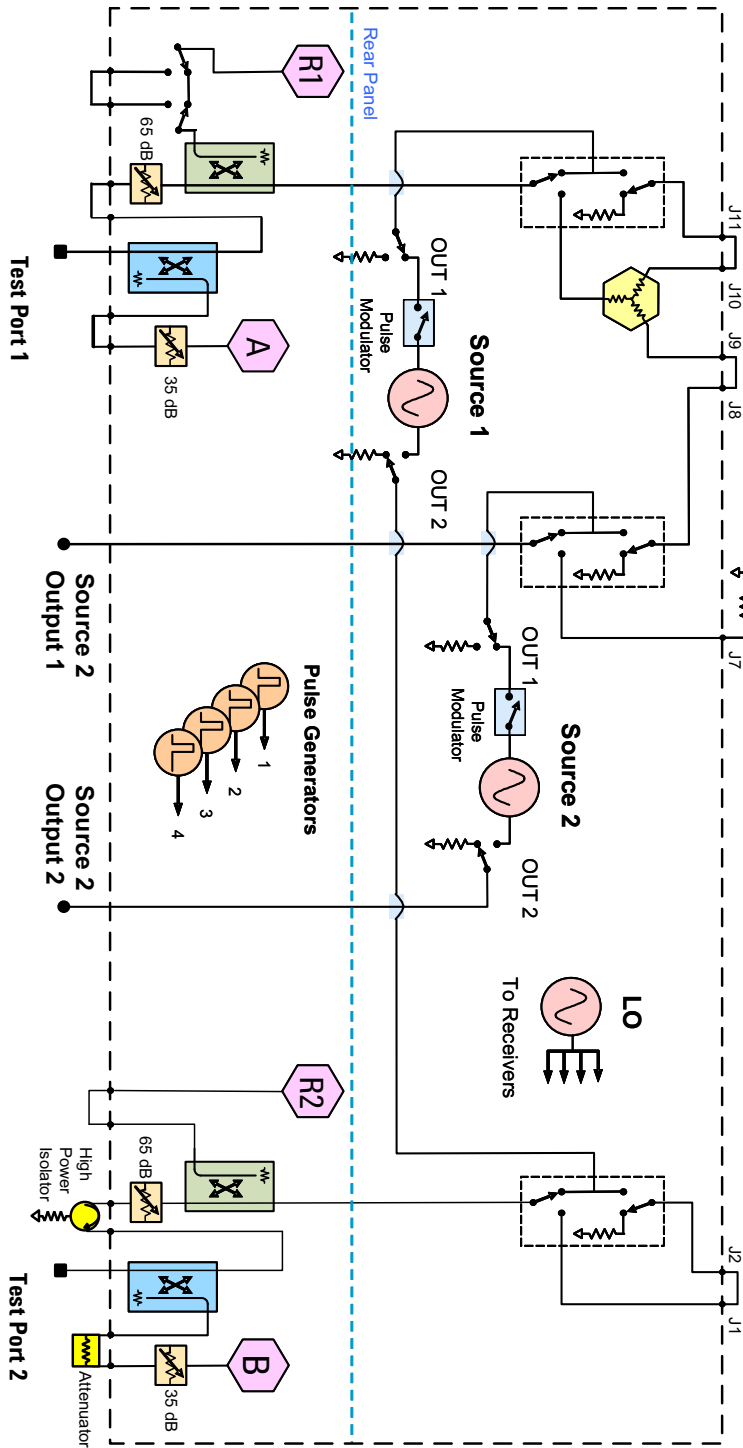

Specifications: Front Panel Jumpers and Test Ports

Specifications for Option H85 are the same as the standard PNA-X with Option 219 or 419. The following specifications are available from the PNA-X Data Sheet at our web site:


<http://www.agilent.com/find/pna>

- Measurement Receiver Inputs
- R1 Reference Receiver Inputs
- R2 - R4 Reference Receiver Inputs
- R1 Source Outputs
- R2 - R4 Source Outputs
- Source Outputs
- Coupler Inputs¹
- Coupler Outputs
- Test Port Inputs

CAUTION It is recommend that you do not operate components near damage or maximum levels. The power levels should be kept at less than 3 dB, preferably 6 dB, below damage and maximum levels.

All PNA-X options have the following front panel jumpers for each port.

Figure 20 Front Panel Jumpers

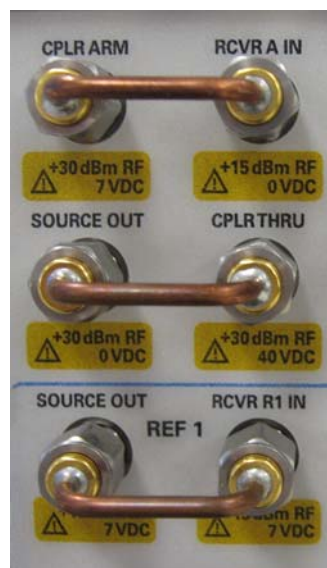

1. Port 1 through Port 4 Insertion Loss of Coupler Thru specifications are the same as the standard Option 200 or 400. Refer to the Agilent 2-Port and 4-Port PNA-X Network Analyzer Data Sheet and Technical Specifications (N5245-90008). The maximum DC Level is 0 VDC.

NOTE Refer to your PNA-X specifications to optimize the power levels in the receivers.

The following tables specify the receiver damage levels for the N5244/45AS Option H85.

Table 1 Damage Power Levels

Measurement Receiver Inputs:	
RCVR A IN through RCVR D IN @ 0.1 dB Typical Compression	
Damage Level	+15 dBm
Maximum DC Level	0 V
R1 Reference Receiver Inputs:	
RCVR R1 IN @ Max Specified Output Power	
Damage Level	+15 dBm
Maximum DC Level	±7 V
R2 - R4 Reference Receiver Inputs:	
RCVR R2 IN through RCVR R4 IN @ Max Specified Output Power	
Damage Level	+15 dBm
Maximum DC Level	± 15 V
R1 Source Outputs:	
Ref 1 Source Out @ Max Specified Output Power	
Damage Level	+15 dBm
Maximum DC Level	± 7 V
R2 - R4 Source Outputs:	
Ref 2 Source Out through Ref 4 @ Max Specified Output Power	
Damage Level	+15 dBm
Maximum DC Level	0 V
Source Outputs:	
Port 1 Source Out through Port 4 @ Max Specified Output Power	
Damage Level	+30 dBm
Maximum DC Level	0 V
Coupler Inputs:	
Port 1 CPLR THRU through Port 4 @ Insertion Loss of Coupler Thru	
Damage Level	+43 dBm
Maximum DC Level	0 V

Table 1 Damage Power Levels

Coupler Outputs:	
Port 1 CPLR ARM through Port 4 @ Max Specified Output Power	
Damage Input Level	+30 dBm
Maximum DC Level	± 7 V
Test Port Inputs:	
Test Port 1 through Port 4 @ Max Specified Output Power	
Damage Level	+43 dBm (without jumpers) +30 dBm (with jumpers)
Maximum DC Level	0 V

Table 2 Watts to dBm Reference Table

Linear (watts)	Log (dBm)
0.001	+0
0.01	+10
0.1	+20
1	+30
2	+33
4	+36
10	+40
20	+43
40	+46
50	+47
100	+50
200	+53

Table 3 Frequency Band-Crossing

Band	Mixer Brick L.O. Harmonic Number	(1)	(2)	(3)	(4)	(5)
		A15 Synthesizer Frequency (GHz)	A25 HMA26.5 Frequency (GHz)	A4/A17 Synthesizer Frequency (GHz)	A5/A10 Source Frequency (GHz)	A7/A8/A12/A13 50 GHz Doubler Frequency (GHz)
0	-	-	-	-	-	-
1	-	-	-	-	-	-
2	1	0.01254 to 0.01654	0.01254 to 0.01654	0.010 to 0.014	0.010 to 0.014	0.010 to 0.014
3	1	0.01654 to 0.02154	0.01654 to 0.02154	0.014 to 0.019	0.014 to 0.019	0.014 to 0.019
4	1	0.02154 to 0.02954	0.02154 to 0.02954	0.019 to 0.027	0.019 to 0.027	0.019 to 0.027
5	1	0.02954 to 0.04054	0.02954 to 0.04054	0.027 to 0.038	0.027 to 0.038	0.027 to 0.038
6	1	0.04054 to 0.05554	0.04054 to 0.05554	0.038 to 0.053	0.038 to 0.053	0.038 to 0.053
7	1	0.06061 to 0.08261	0.06061 to 0.08261	0.053 to 0.075	0.053 to 0.075	0.053 to 0.075
8	1	0.08261 to 0.11261	0.08261 to 0.11261	0.075 to 0.105	0.075 to 0.105	0.075 to 0.105
9	1	0.11261 to 0.15361	0.11261 to 0.15361	0.105 to 0.146	0.105 to 0.146	0.105 to 0.146
10	1	0.15361 to 0.21261	0.15361 to 0.21261	0.146 to 0.205	0.146 to 0.205	0.146 to 0.205
11	1	0.21261 to 0.25761	0.21261 to 0.25761	0.205 to 0.250	0.205 to 0.250	0.205 to 0.250
12	1	0.25761 to 0.40361	0.25761 to 0.40361	0.250 to 0.396	0.250 to 0.396	0.250 to 0.396
13	1	0.40361 to 0.50761	0.40361 to 0.50761	0.396 to 0.500	0.396 to 0.500	0.396 to 0.500
14	1	0.50761 to 0.63561	0.50761 to 0.63561	0.500 to 0.628	0.500 to 0.628	0.500 to 0.628
15	1	0.63561 to 1.00761	0.63561 to 1.00761	0.628 to 1.000	0.628 to 1.000	0.628 to 1.000
16	1	1.00761 to 1.50761	1.00761 to 1.50761	1.000 to 1.500	1.000 to 1.500	1.000 to 1.500
17	1	1.50761 to 2.00761	1.50761 to 2.00761	1.500 to 2.000	1.500 to 2.000	1.500 to 2.000
18	1	2.00761 to 3.00761	2.00761 to 3.00761	2.000 to 3.000	2.000 to 3.000	2.000 to 3.000
19	1	3.00761 to 3.20761	3.00761 to 3.20761	3.000 to 3.200	3.000 to 3.200	3.000 to 3.200
20	1	3.20761 to 4.00761	3.20761 to 4.00761	3.200 to 4.000	3.200 to 4.000	3.200 to 4.000
21	1	4.00761 to 5.33961	4.00761 to 5.33961	4.000 to 5.332	4.000 to 5.332	4.000 to 5.332
22	1	5.33961 to 6.75961	5.33961 to 6.75961	5.332 to 6.752	5.332 to 6.752	5.332 to 6.752
23	1	6.75961 to 8.00761	6.75961 to 8.00761	6.752 to 8.000	6.752 to 8.000	6.752 to 8.000
24	1	8.00761 to 8.50761	8.00761 to 8.50761	8.000 to 8.500	8.000 to 8.500	8.000 to 8.500
25	1	8.50761 to 10.67161	8.50761 to 10.67161	8.500 to 10.664	8.500 to 10.664	8.500 to 10.664
26	1	10.67161 to 12.00761	10.67161 to 12.00761	10.664 to 12.000	10.664 to 12.000	10.664 to 12.000
27	1	12.00761 to 12.80761	12.00761 to 12.80761	12.000 to 12.800	12.000 to 12.800	12.000 to 12.800
28	1	12.80761 to 13.51761	12.80761 to 13.51761	12.800 to 13.510	12.800 to 13.510	12.800 to 13.510
29	1	6.75880 to 7.70380	13.51761 to 15.40761	6.755 to 7.700	13.510 to 15.400	13.510 to 15.400
30	1	7.70380 to 8.00380	15.40761 to 16.00761	7.700 to 8.000	15.400 to 16.000	15.400 to 16.000
31	1	8.00380 to 9.50380	16.00761 to 19.00761	8.000 to 9.500	16.000 to 19.000	16.000 to 19.000
32	1	9.50380 to 10.00380	19.00761 to 20.00761	9.500 to 10.000	9.500 to 10.000	19.000 to 20.000
33	1	10.00380 to 10.66781	20.00761 to 21.33561	10.000 to 10.664	10.000 to 10.664	20.000 to 21.328
34	1	10.66781 to 12.00381	21.33561 to 24.00761	10.664 to 12.000	10.664 to 12.000	21.328 to 24.000
35	1	12.00381 to 13.25381	24.00761 to 26.50761	12.000 to 13.250	12.000 to 13.250	24.000 to 26.500
36	3	8.83587 to 9.00520	8.83587 to 9.00520	13.250 to 13.504	13.250 to 13.504	26.500 to 27.008
37	3	9.00520 to 10.66920	9.00520 to 10.66920	6.752 to 8.000	13.504 to 16.000	27.008 to 32.000
38	3	10.66920 to 12.16920	10.66920 to 12.16920	8.000 to 9.125	16.000 to 18.250	32.000 to 36.500
39	3	12.16920 to 13.50254	12.16920 to 13.50254	9.125 to 10.125	18.250 to 20.250	36.500 to 40.500
40	3	6.75127 to 7.11060	13.50254 to 14.22120	10.125 to 10.664	20.250 to 21.328	40.500 to 42.656
41	3	7.11060 to 7.25127	14.22120 to 14.50254	10.664 to 10.875	21.328 to 21.750	42.656 to 43.500
42	3	7.25127 to 7.70127	14.50254 to 15.40254	10.875 to 11.550	21.750 to 23.100	43.500 to 46.200
43	3	7.70127 to 8.00127	15.40254 to 16.00254	11.550 to 12.000	23.100 to 24.000	46.200 to 48.000
44	3	8.00127 to 8.33460	16.00254 to 16.66920	12.000 to 12.500	24.000 to 25.000	48.000 to 50.000

Example: Making High Power Measurements With Option H85

This section describes how to set up the analyzer to perform high power measurements. Analyzers equipped with the Option H85 can be configured to measure high power devices. This ability is useful if the required power for the device under test is greater than the analyzer can provide, or if the maximum output power from an amplifier under test exceeds safe input limits for a standard analyzer.

This 2-Port example of the high power procedure chooses an optimal power level of -12 dBm for all receivers. You may choose to optimize your measurement performance by using [Table 1 on page 21](#).

Typeface Key Conventions


The following key conventions are used throughout this document.

- **[HARDKEYS]** are labeled front panel keys.
- **SOFTKEYS** are unlabeled key whose function is indicated on the instrument display.

Initial Setup

1. If the analyzer is in the standard mode configuration remove the jumper between Port 1 SOURCE OUT and CPLR THRU connector on the front panel. This can also be done for Port 2 if high power measurements are necessary for the reverse parameters of a device under test (DUT). Two booster amplifiers and two 20 dB couplers are required for both forward and reverse measurements. Refer to [Figure 21](#).
2. Connect the booster amplifier RF INPUT connector to the Port 1 SOURCE OUT connector on the front panel of the analyzer.
3. Connect a 20 dB coupler (that operates within the frequency range of interest) to the booster amplifier RF OUTPUT connector.

Figure 21 Booster Amplifier and 20 dB Coupler Connection Setup

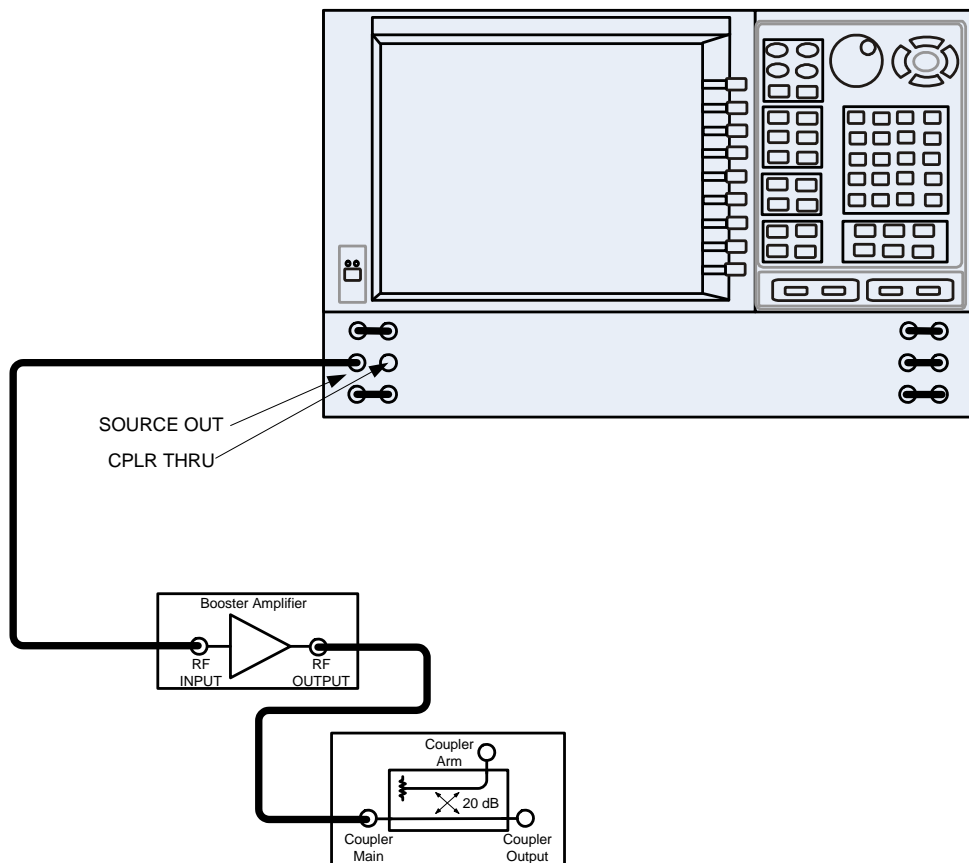


Determining Power Levels

NOTE For all high power configurations refer to [Table 1 on page 21](#) for maximum input damage levels, and PNA-X specifications to optimize the power levels on the receivers.

Before continuing, save this state and set it up as the **User Preset**. The User Preset Conditions can be found in the PNA-X Series Network Analyzer's help menu.

1. Press **[Help]** on the front panel, or in the **Help** drop-down menu select **Network Analyzer Help**. Type **User Preset** in the index or search field and select **Display**. This will describe how to setup a User Preset. The final state should be saved as the User Preset to avoid an over power condition from the factory preset.

Figure 22 Help Menu

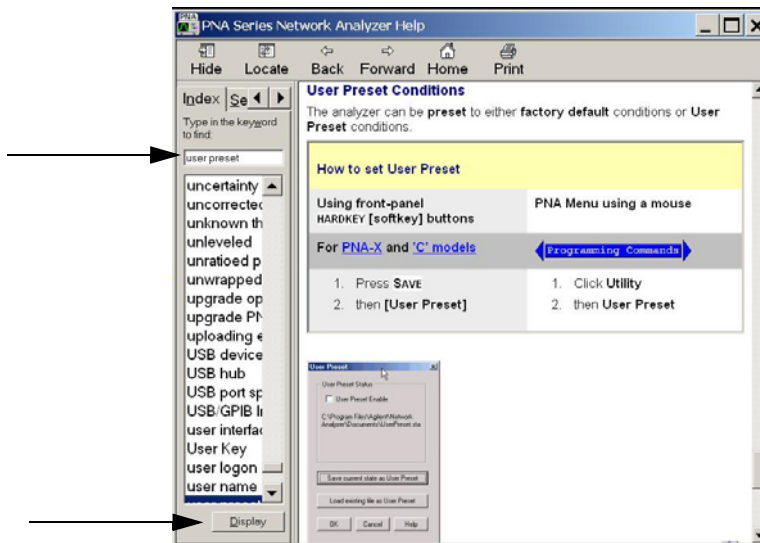


Example: Making High Power Measurements With Option H85

To find the User Preset:


- In the **Utility** drop-down menu select **User Preset**. Check **User Preset Enable** > **Save current state as User Preset** and press **OK**. See [Figure 23](#).

Figure 23 User Preset

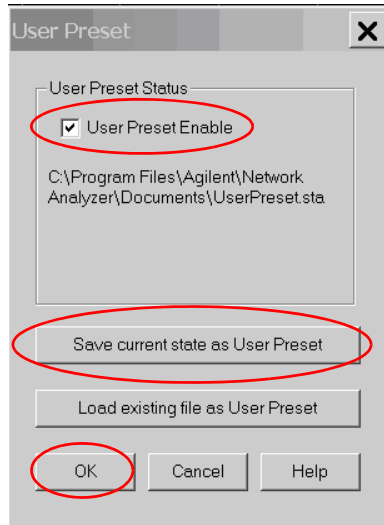

- In the **Stimulus** drop-down menu select **Power** > **Power and Attenuators**. In the dialog box type **[-20 dBm]** into **Port Power** for **Port 1**. Verify that **Port Powers Coupled** is checked to ensure that Ports 1 and Port 2 power levels are the same. Press **OK**. Uncoupled ports should be used when adjusting the S12 power level. See [Figure 24](#).

Figure 24 Power and Attenuators

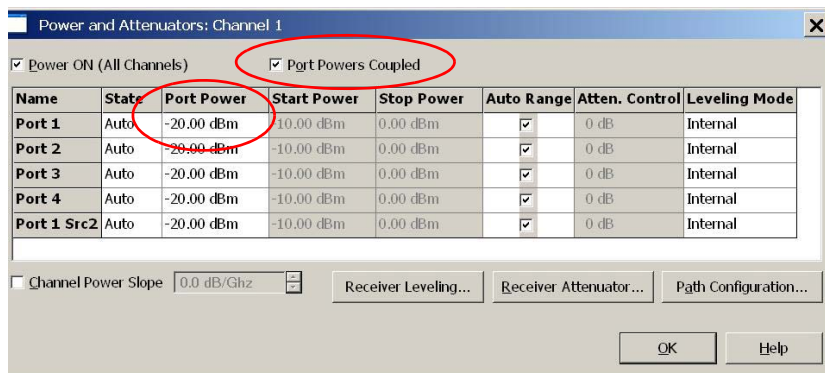

Example: Making High Power Measurements With Option H85

4. Turn On the booster amplifier.
5. Measure the output power from the coupled arm and the open port “Coupler Output” of the coupler, using a power meter and sensor.


NOTE Depending on the power used, additional attenuation may have to be added between the coupler and the power meter.

6. Verify the gain of the booster amplifier(s). For example; if the analyzer output power level was set to -20 dBm and the output power measured from the open end of the coupler was -5 dBm, the gain of the booster amplifier would be $+15$ dB.
7. Verify that the power measured in the previous steps is within the acceptable limits (less than -12 dBm for the coupled arm, less than $+43$ dBm for the open port). Estimate the maximum power level needed to force the DUT into compression.
8. At the maximum estimated power level, determine if the maximum output power from the coupled arm of the coupler will be higher than the acceptable limit. If so, add the appropriate amount of attenuation that will keep the coupler arm output power below -12 dBm.

Additional Setup

9. Turn Off the booster amplifier.
10. Connect the open port of the 20 dB coupler to the Port 1 CPLR THRU connector on the front panel. This can also be done on Port 2 if reverse parameters high power measurements are required.
11. Disconnect the REFERENCE SOURCE OUT and RCVR R1 IN jumper on the front panel. Connect the coupled arm of the 20 dB coupler (along with any added attenuation) to the RCVR R1 IN. The same instructions apply to Port 2 with one exception; disconnect the jumper to RCVR R2 IN if high power measurements are required for the reverse parameters.


Figure 25 PNA-X Port 1 Amplifier, Coupler, Attenuator Connections

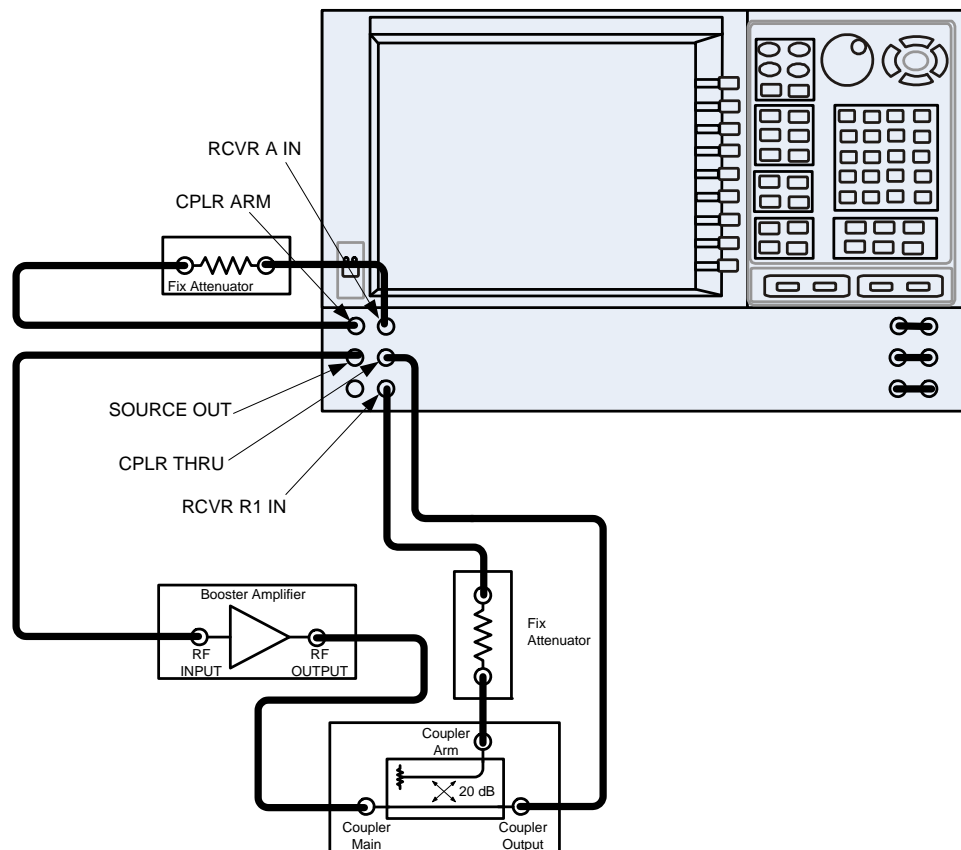

Selecting Power Ranges and Attenuator Settings

12. Select a power range that will not exceed the maximum estimated power level, but will force the DUT into compression. For example; if your booster amplifier has a gain of +15 dB, the DUT will compress if supplied with +15 dBm. You may need to adjust the analyzer output power to not exceed 0 dBm.
13. In the **Stimulus** drop-down menu select **Power > Power and Attenuators**. In the dialog box, clear the **Auto Range** box and type [10 dB] into **Atten. Control** for **Port 1**. Verify that **Port Powers Coupled** is checked to ensure that Ports 1 and Port 2 power levels are the same. Press **OK**.


Figure 26 Attenuator Control

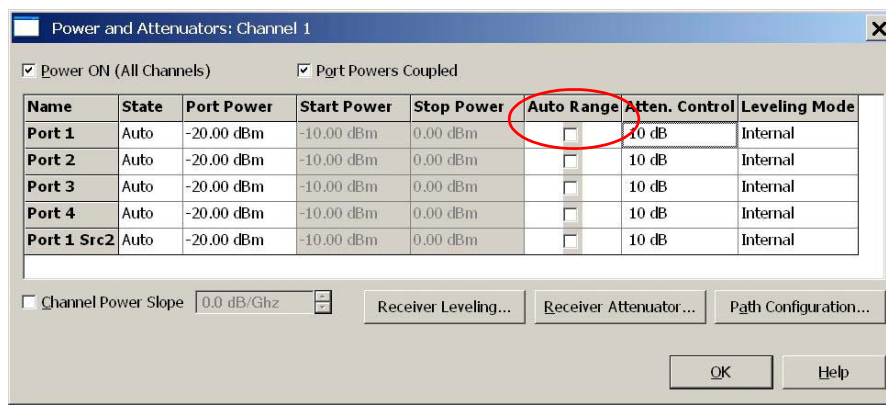

Example: Making High Power Measurements With Option H85

14. Estimate the maximum amount of gain that could be provided by the DUT, and as a result, the maximum amount of power that could be received by Test Port 2 when the DUT is in compression. For example; if a DUT with a maximum gain of +10 dB receives an input of +10 dBm, the maximum amount of power that could be received by Test Port 2 is +20 dBm. An isolator or attenuator may be required depending on the amount of power at Test Port 2. For Port 2 isolators and attenuator connections, an isolator is placed between the CPLR THRU and SOURCE OUT as shown in Figure 27.

Figure 27 Isolators and Attenuator Connections

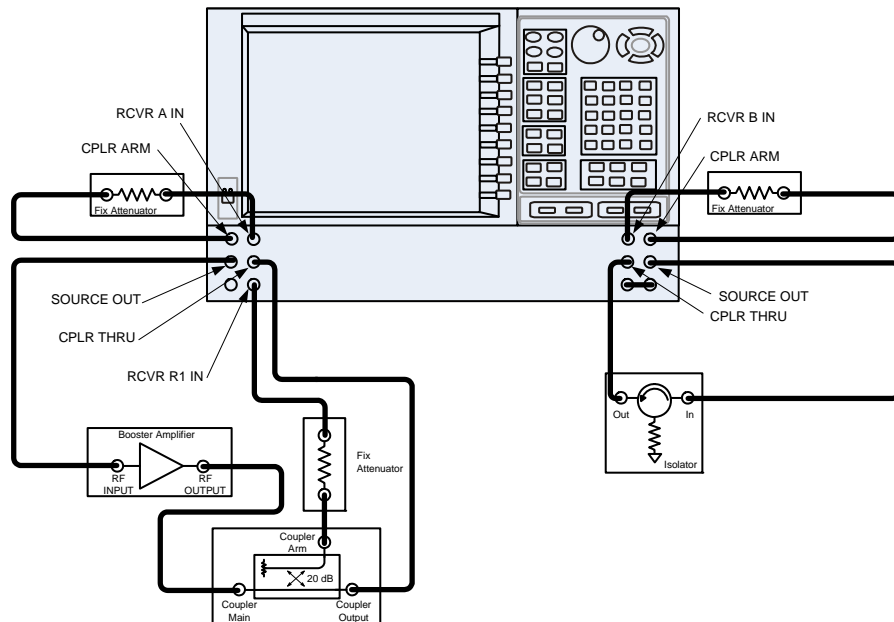

15. Calculate the amount of attenuation needed between the analyzer's coupler and receivers, so that you do not exceed the optimum receiver power level of -12 dBm.

It will be necessary to take the following into consideration:

- Receiver A will be coupled to the analyzer RF path that could receive power reflections as high as +10 dBm.
- Receiver B will be coupled to the analyzer RF path that could receive a maximum of +20 dBm from the DUT.
- Analyzer coupler loss is -13 dB.
- The optimum receiver power level is -12 dBm.


With the previous points in mind, the amount of attenuation can be calculated from the following equations:

$$\text{Receiver Attenuator A} = +10\text{dBm} - 13\text{dBm} - (-12\text{dBm}) \quad \text{Attenuator A} = +10\text{dBm}$$

$$\text{Receiver Attenuator B} = +20\text{dBm} - 13\text{dBm} - (-12\text{dBm}) \quad \text{Attenuator B} = +20\text{dBm}$$

Example: Making High Power Measurements With Option H85


16. Set the receiver attenuator to the value calculated in the previous step (rounding off to the highest 5 dB step). Setting the receiver attenuation will establish the internal attenuation. In the **Stimulus** drop-down menu select **Power > Power and Attenuators**. In the dialog box, select **Receiver Attenuators**. Set Receiver A to **[10 dB]** and Receiver B to **[20 dB]** and select **OK**, see [Figure 28](#). Power levels greater than +35 dBm will require additional attenuation between Port 2 access ports CPLR ARM and RCVR B IN, see [Figure 27 on page 31](#).

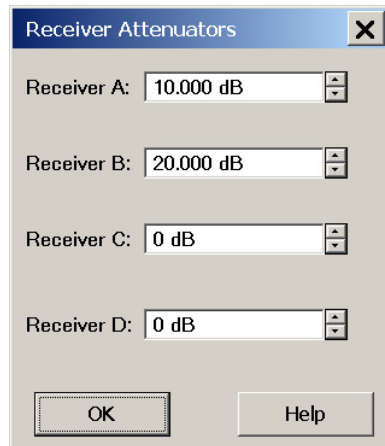Figure 28 Receiver Attenuators

17. Turn On the booster amplifier.

CAUTION From this point forward, *do not* press Preset unless you have turned off the booster amplifier(s), or have renamed and saved this state as User Preset. Pressing Preset will return the analyzer to its default power level and default internal attenuator settings. This increase in power may result in damage to the DUT or analyzer.


18. In the **Trace/Chan** drop-down menu select **Channel > Hardware Setup > Path Config**.

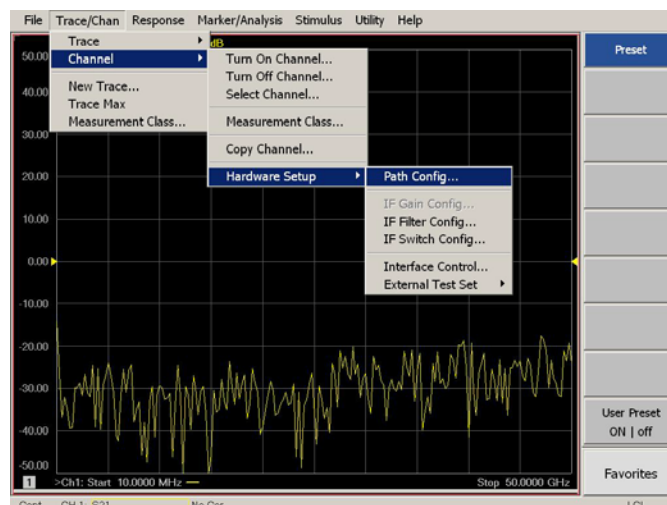Figure 29 Path Configuration

Example: Making High Power Measurements With Option H85

19. In the dialog box, select **Port 1 Reference Mixer Switch** > **External** and press **OK** to active the R1 Input path.

Figure 30 Port 1 Mixer Switch

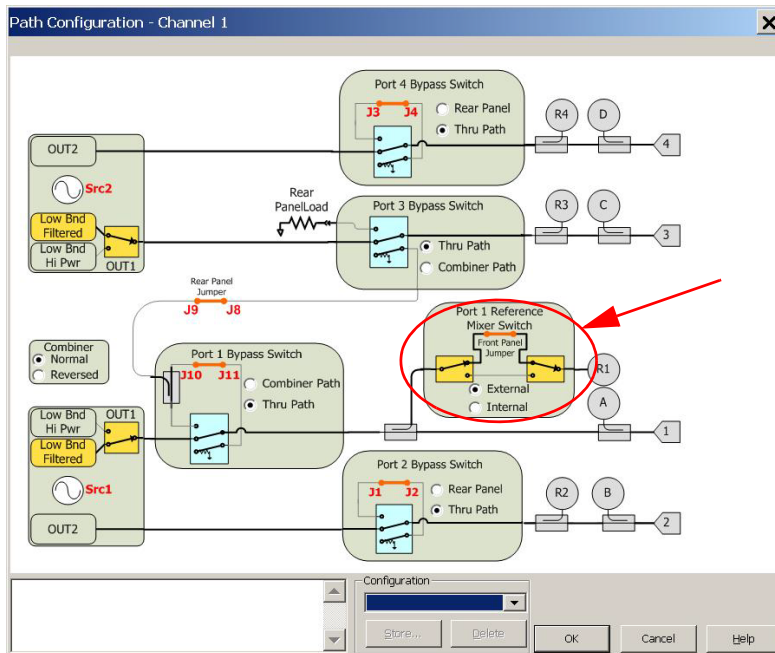

20. Measure the output power at Test Port 1, using a power meter. Verify the power measurement.


If you are measuring a highly reflective device, a high power isolators should be inserted between the 20 dB coupler and CPLR THRU front panel ports to protect Port 1 Source.

Final Setup

21. Verify that all of the power and attenuator settings are correct.

22. In the **Response** drop-down menu select **Measure > S21**.


Figure 31 Response Menu

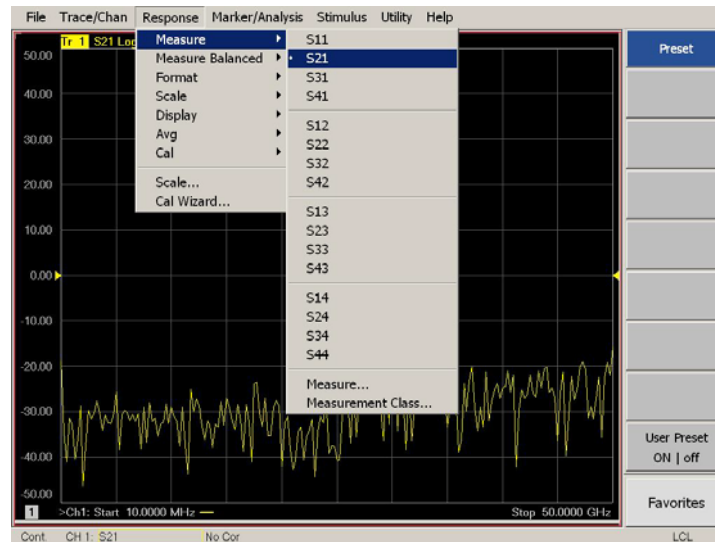

23. To Perform a response calibration following steps a, b, c and d:

- a. Connect the test port cables of the analyzer to form a thru configuration.
- b. In the **Response** drop-down menu select **Cal Wizard** (see [Figure 31](#)). In the dialog box, select **UNGUIDED Calibration (Response, 1-port 2-port): Use Mechanical Standards > Next**.


Figure 32 Calibration Wizard

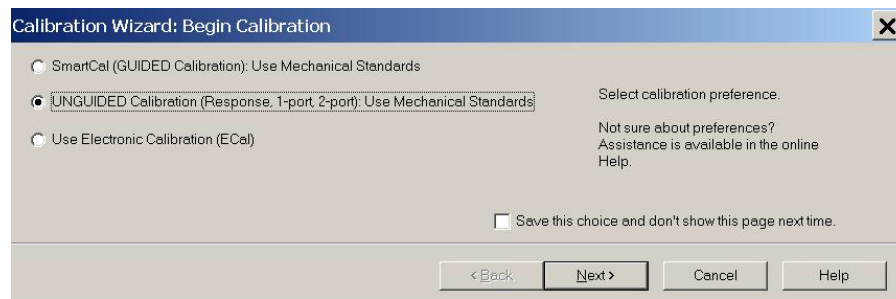

Example: Making High Power Measurements With Option H85


- c. Select **Response** > **Next**.

Figure 33 **Response**

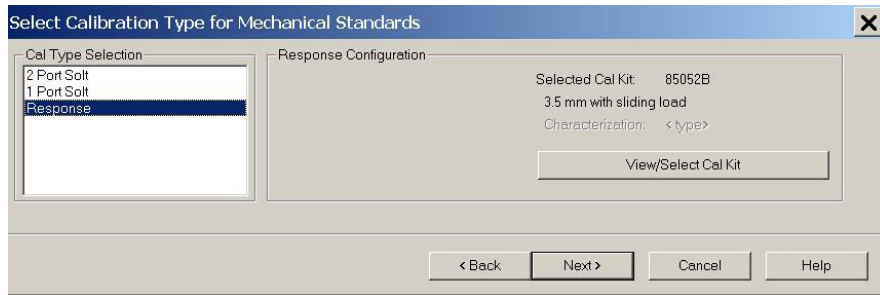


- d. Select **THRU** > **Next**. Follow the analyzers window prompts to finish calibration.

Figure 34 **THRU**

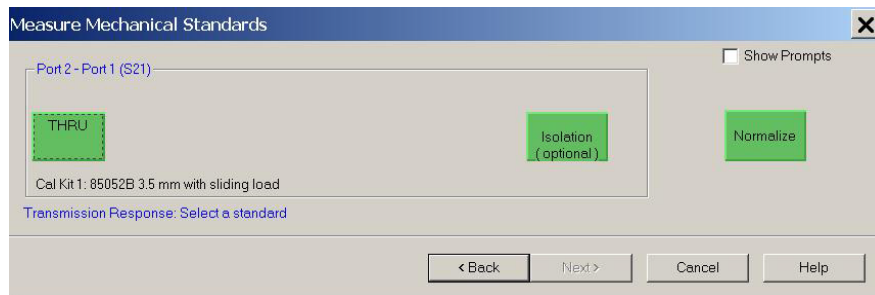

24. Configure the test setup as shown in [Figure 35](#). Turn On the DUT and measure the **S21** gain of the amplifier under test to confirm the proper operation of the measurement test setup.

Figure 35 Forward High Power Measurement Configuration

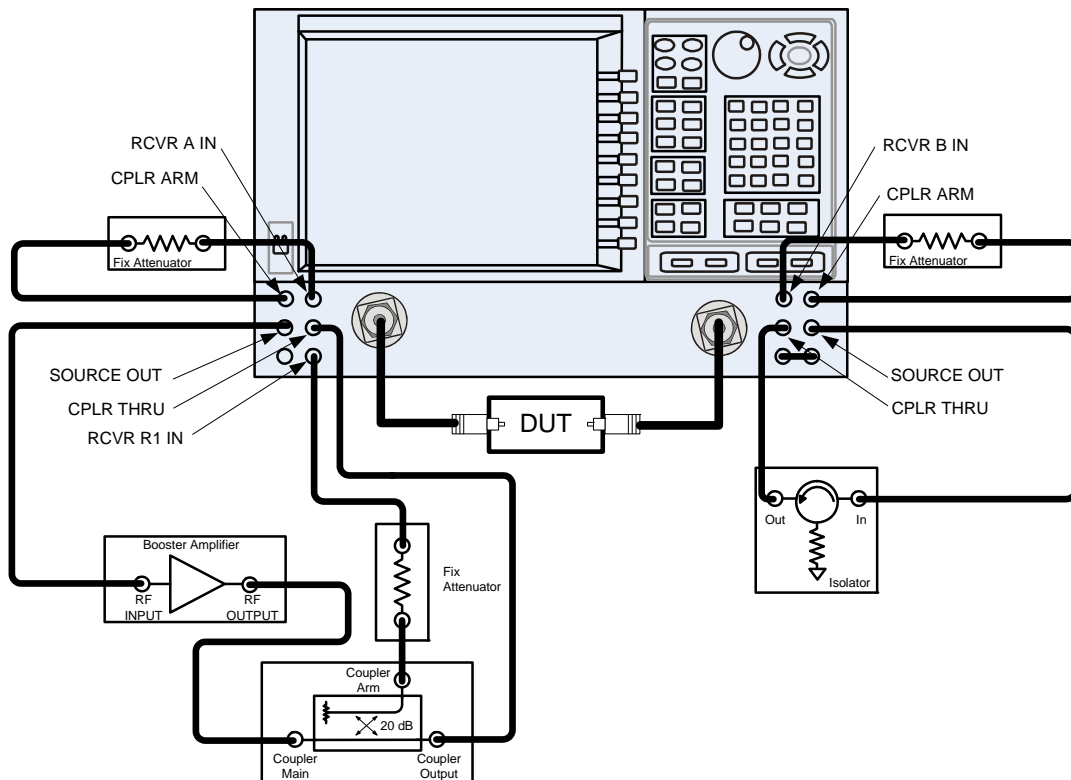

25. Continue with any other high power measurements.

NOTE Ratio measurements, such as gain, will be correctly displayed. However, the displayed absolute power levels on the analyzer will *not* be correct. To correctly interpret power levels and the gain of the booster amplifier, the attenuator setting must be taken into consideration.

If no calibration has been performed or if the instrument is in an un-calibrated state, the following must be taken into consideration when interpreting the measured data:

- The value of attenuation added to receiver A and B.
- The R channel reference level supplied from the coupler arm of the 20 dB coupler.

This procedure can be repeated to setup the reverse high power configuration.

Specification

The N5244/45AS models are tested to the performance closest matching their configuration. Specifications for the N5244/45AS with Option H85 (Delete Bias Tees) are equivalent to the N5244/45A with Options 200/219 (2-Port PNA-X, Source/Receiver Attens + Bias Tees) or Options 400/419 (4-Port PNA-X, Source/Receiver Attens + Bias Tees). Deviations from these specifications are documented in this manual.

Specifications are both viewable and printable from the PNA-X Series Data Sheet. Visit our web site at <http://www.agilent.com/find/pna>, enter your analyzer model number (N5244/45A) in the search field and select the data sheet or manual of your choice.

The specifications for Option H85, when configured in high power or large signal capability, are not tested nor guaranteed.

Service Information

Information can be found in the Agilent 2-Port and 4-Port PNA-X Network Analyzer Data Sheet and Technical Specifications (N5245-90008). This document can be found using the our web site at <http://www.agilent.com/find/pna>, enter N5245-90008 in the search field.

Service information can be found in the Agilent N5244A and N5245A 2-Port and 4-Port PNA Microwave Network Analyzers Service Guide (N5245-90001). This document can be found using the our web site at <http://www.agilent.com/find/pna>, enter N5245-90001 in the search field. Replacement parts and procedures are listed in Chapters 6 & 7.

The Agilent Technologies PNA-X Series Microwave Network Analyzers N5244/45A will display Option H85. Firmware revision A.08.60.07 or higher must be used for this option. Service software is available for servicing the N5244/45A at local service centers.

Follow the N5244/45A Service Guide instructions for all repair, replacement procedures, tests and adjustments.

Replaceable Parts

NOTE Special options are built to order, so long lead times may be encountered when ordering replacement parts.

Reference Designator	PNA-X	Description	Agilent Part Number
Add:			
W20	N5244/45A-200	RF Cable: Port 1 CPLR THRU to A33 Port 1 Coupler	N5245-20045
W32	N5244/45A-200	RF Cable: Port 2 CPLR THRU to A36 Port 2 Coupler	N5245-20106
W20	N5244/45A-400	RF Cable: Port 1 CPLR THRU to A33 Port 1 Coupler	N5245-20099
W24	N5244/45A-400	RF Cable: Port 3 CPLR THRU to A34 Port 3 Coupler	N5245-20098
W28	N5244/45A-400	RF Cable: Port 4 CPLR THRU to A35 Port 4 Coupler	N5245-20096
W32	N5244/45A-400	RF Cable: Port 2 CPLR THRU to A36 Port 2 Coupler	N5245-20097
	N5244/45A-200/219	Front Panel Overlay, 2-Port (Option H85)	N5242-80014
	N5244/45A-200/219/224	Front Panel Overlay, 2-Port (Option H85/224)	N5245-80013
	N5244/45A-400/419/423	Front Panel Overlay, 4-Port (Option H85)	N5242-80016
Delete:			
A42/A45	N5244/45A-219	Bias-tee with wire harness	5087-7331
A42/A43A/44/A45	N5244/45A-419	Bias-tee with wire harness	5087-7331
W83	N5244/45A-219	RF Cable: Front Panel Port 1 CPLR THRU to A42 Port 1 Bias-Tee	N5245-20046
W84	All	RF Cable: A33 Port 1 Coupler to A42 Port 1 Bias-Tee	N5245-20076
W95	N5244/45A-219	RF Cable: Front Panel Port 2 CPLR THRU to A45 Port 2 Bias-Tee	N5245-20047
W96	All	RF Cable: A36 Port 2 Coupler to A45 Port 2 Bias-Tee	N5245-20030
W83	N5244/45A-419	RF Cable: Front Panel Port 1 CPLR THRU to A42 Port 1 Bias-Tee	N5245-20085
W95	N5244/45A-419	RF Cable: Port 2 CPLR THRU to A45 Port 2 Bias-Tee	N5245-20087
W87	N5244/45A-419	RF Cable: Port 3 CPLR THRU to A43 Port 3 Bias-Tee	N5245-20089

Reference Designator	PNA-X	Description	Agilent Part Number
W88	N5244/45A-419	RF Cable: A43 Port 3 Bias-Tee to A34 Port 3 Coupler	N5245-20086
W91	N5244/45A-419	RF Cable: Port 4 CPLR THRU to A44 Port 4 Bias-Tee	N5245-20090
W92	N5244/45A-419	RF Cable: A44 Port 4 Bias-Tee to A35 Port 4 Coupler	N5245-20088
	N5244/45A-200/219	Front Panel Overlay, 2-Port (Option 200/219)	N5242-80001
	N5244/45A-200/219/224	Front Panel Overlay, 2-Port (Option 224)	N5245-80005
	N5244/45A-400/419/423	Front Panel Overlay, 4-Port (All Options)	N5242-80003

Safety and Regulatory Information

Introduction

Review this product and related documentation to familiarize yourself with safety markings and instructions before you operate the instrument. The documentation contains information and warnings that must be followed by the user to ensure safe operation and to maintain the product in a safe condition.

Before Applying Power

Verify that the premises electrical supply is within the range of the instrument. The instrument has an autoranging power supply.

WARNING To prevent electrical shock, disconnect the **Agilent Technologies N5244/45AS Option H85** from mains electrical supply before cleaning. Use a dry cloth or one slightly dampened with water to clean the external case parts. Do not attempt to clean internally.

Connector Care and Cleaning

If alcohol is used to clean the connectors, the power cord to the instrument must be removed. All cleaning should take place in a well ventilated area. Allow adequate time for the fumes to disperse and moist alcohol to evaporate prior to energizing the instrument.

WARNING Keep isopropyl alcohol away from heat, sparks, and flame. Store in a tightly closed container. It is extremely flammable. In case of fire, use alcohol foam, dry chemical, or carbon dioxide; water may be ineffective.

Declaration of Conformity

A declaration of conformity is on file for the PNA-X models, and a copy is available upon request, or a copy is available on the Agilent Technologies web site at <http://prodregs.corporate.agilent.com>

Statement of Compliance

This instrument has been designed and tested in accordance with IEC 61010-1 (2nd Edition) and has been supplied in a safe condition. The instruction documentation contains information and warnings which must be followed by the user to ensure safe operation and to maintain the instrument in a safe condition.

General Safety Considerations

Safety Earth Ground

WARNING This is a Safety Class I product (provided with a protective earthing ground incorporated in the power cord). The mains plug shall only be inserted in a socket outlet provided with a protective earth contact. Any interruption of the protective conductor, inside or outside of the instrument, will make the instrument dangerous. Intentional interruption is prohibited.

Cautions applicable this instrument.

CAUTION Always use the three-prong ac power cord supplied with this instrument. Failure to ensure adequate earth grounding (by not using this cord) can cause instrument damage and the risk of electrical shock.

CAUTION This product is designed for use in Installation Category II and Pollution Degree 2.

CAUTION This instrument has autoranging line voltage input; be sure the supply voltage is within the specified range.

CAUTION Ventilation Requirements: When installing the instrument in a cabinet, the convection into and out of the instrument must not be restricted. The ambient temperature (outside the cabinet) must be less than the maximum operating temperature of the instrument by 4 °C for every 100 watts dissipated in the cabinet. If the total power dissipated in the cabinet is greater than 800 watts, forced convection must be used.

Servicing

Warnings applicable to this instrument.

WARNING This is a Safety Class I product (provided with a protective earthing ground incorporated in the power cord). The mains plug shall be inserted only into a socket outlet provided with a protective earth contact. Any interruption of the protective conductor, inside or outside the product is likely to make the product dangerous. Intentional interruption is prohibited.

WARNING These servicing instructions are for use by qualified personnel only.

WARNING The opening of covers or removal of parts is likely to expose the user to dangerous voltages. Disconnect the instrument from all voltage sources while it is being opened.

WARNING This product is designed for use in Installation Category II and Pollution Degree 2.

WARNING No operator serviceable parts inside. Refer servicing to qualified personnel.

WARNING If this product is not used as specified, the protection provided by the equipment could be impaired. This product must be used in a normal condition (in which all means for protection are intact) only.

NOTE There are no operator replaceable fuses in the mains input.

Regulatory Information

This section contains information that is required by various government regulatory agencies.

Instrument Markings



The instruction documentation symbol. The product is marked with this symbol when it is necessary for the user to refer to the instructions in the documentation.



This symbol indicates that the instrument requires alternating current (ac) input.



This symbol indicates separate collection for electrical and electronic equipment, mandated under EU law as of August 13, 2005. All electric and electronic equipment are required to be separated from normal waste for disposal (Reference WEEE Directive, 2002/96/EC).



This symbol indicates that the power line switch is ON.



This symbol indicates that the power line switch is in the STANDBY position.



This symbol indicates that the power line switch is in the OFF position.



This symbol is used to identify a terminal which is internally connected to the product frame or chassis.



The CE mark is a registered trademark of the European Community. (If accompanied by a year, it is when the design was proven.)



The CSA mark is a registered trademark of the CSA International. This instrument complies with Canada: CSA 22.2 No. 61010-1-04.



This is a symbol of an Industrial Scientific and Medical Group 1 Class A product.



This is a marking to indicate product compliance with the Canadian Interference-Causing Equipment Standard (ICES-001).



Direct Current.



This is a required mark signifying compliance with an EMC requirement. The C-Tick mark is a registered trademark of the Australian Spectrum Management Agency.



China RoHS regulations include requirements related to packaging, and require compliance to China standard GB18455-2001.



This symbol indicates compliance with the China RoHS regulations for paper/fiberboard packaging.

Compliance with German FTZ Emissions Requirements

This product complies with the German FTZ 526/527 Radiated Emissions and Conducted Emission requirements.

Compliance with German Noise Requirements

This is to declare that this instrument is in conformance with the German Regulation on Noise Declaration for Machines (Laermangabe nach der Maschinenlaermrrordnung-3. GSGV Deutschland).

Acoustic Noise Emission/Geraeuschemission	
LpA<70 dB	Lpa<70 dB
Operator Position	am Arbeitsplatz
Normal Operation	normaler Betrieb
per ISO 7779	nach DIN 45635 t. 19

EMC Information

Complies with European EMC Directive 2004/108/EC

- IEC/EN 61326-1
- CISPR Pub 11 Group 1, class A
- AS/NZS CISPR 11
- This ISM device complies with Canadian ICES-001.
Cet appareil ISM est conforme a la norme NMB du Canada.

Safety Information

Complies with European Low Voltage Directive 2006/95/EC


- IEC/EN 61010-1, 2nd Edition
- Canada: CSA C22.2 No. 61010-1-04
- USA: UL Std. No. 61010-1 (2nd Edition)

Electrostatic Discharge Protection

Protection against electrostatic discharge (ESD) is essential while removing assemblies from or connecting cables to the network analyzer. Static electricity can build up on your body and can easily damage sensitive internal circuit elements when discharged. Static discharges too small to be felt can cause permanent damage. To prevent damage to the instrument:

- *always* have a grounded, conductive table mat (9300-0797) in front of your test equipment.
- *always* wear a grounded wrist strap (9300-1367) with grounding cord (9300-0980), connected to a grounded conductive table mat, having a 1 M Ω resistor in series with it, when handling components and assemblies or when making connections.
- *always* wear a heel strap (9300-1126) when working in an area with a conductive floor. If you are uncertain about the conductivity of your floor, wear a heel strap.
- *always* ground yourself before you clean, inspect, or make a connection to a static-sensitive device or test port. You can, for example, grasp the grounded outer shell of the test port or cable connector briefly.
- *always* ground the center conductor of a test cable before making a connection to the analyzer test port or other static-sensitive device. This can be done as follows:
 1. Connect a short (from your calibration kit) to one end of the cable to short the center conductor to the outer conductor.
 2. While wearing a grounded wrist strap, grasp the outer shell of the cable connector.
 3. Connect the other end of the cable to the test port and remove the short from the cable.

Figure 36 ESD Protection Setup

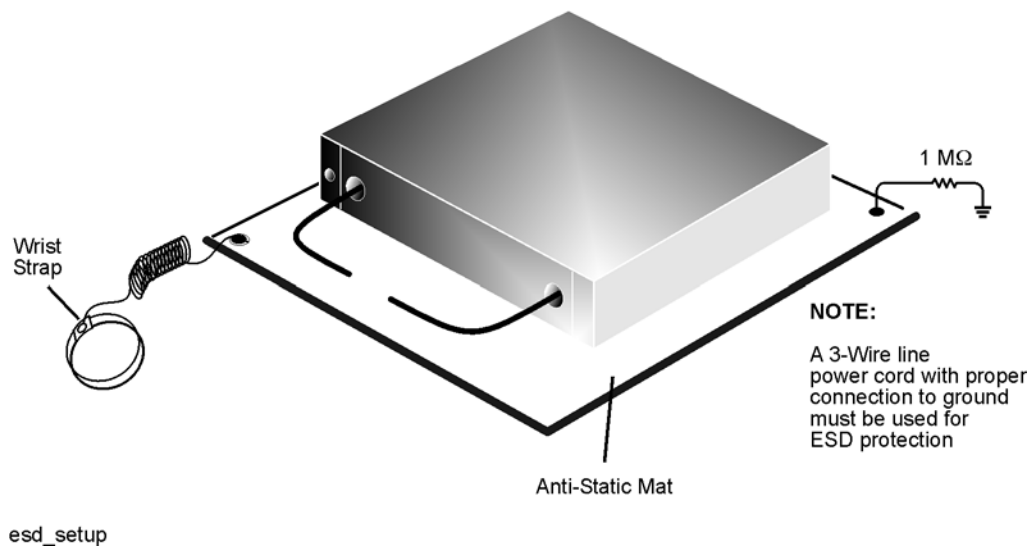

Agilent Support and Assistance

Service and Support Options

The analyzer's standard warranty is a one-year return to Agilent Technologies service warranty.

See “[Service Information](#)” on page 37 for PNA-X information.

NOTE There are many other repair and calibration options available from the Agilent Technologies support organization. These options cover a range of service agreements with varying response times. Contact Agilent for additional information on available service agreements for this product. Refer to “[Contacting Agilent](#)” on page 46.

Contacting Agilent

Assistance with test and measurements needs and information or finding a local Agilent office are available on the Web at:

<http://www.agilent.com/find/assist>

If you do not have access to the Internet, please contact your Agilent field engineer.

NOTE In any correspondence or telephone conversation, refer to the Agilent product by its model number and full serial number. With this information, the Agilent representative can determine whether your product is still within its warranty period.

Shipping Your Analyzer to Agilent for Service or Repair

IMPORTANT Agilent Technologies reserves the right to reformat or replace the internal hard disk drive in your analyzer as part of its repair. This will erase all user information stored on the hard disk. It is imperative, therefore, that you make a backup copy of your critical test data located on the analyzer's hard disk before shipping it to Agilent for repair.

If you wish to send your network analyzer to Agilent Technologies for service or repair:

- Include a complete description of the service requested or of the failure and a description of any failed test and any error message.
- Ship the analyzer using the original or comparable antistatic packaging materials.
- Contact Agilent for instructions on where to ship your analyzer.