
Getting Started Guide

HP 1650B/HP 1651 B Logic Analyzers

OTS LIBRARY



OTS LIBRARY



2400010748

©Copyright Hewlett-Packard Company 1989

Manual Part Number 5952-4240

Printed in the USA. July 1989

01650-90914

Contents

Introduction

About this book . . .

Chapter 1:

Introducing the **HP1650B/HP 1651B**

What Are the HP 1650B and HP 1651B?	1-1
Getting Ready to Operate	1-2
Initial Inspection	1-2
Accessories	1-3
Removing Yellow Shipping Disc	1-3
Selecting the Line Voltage	1-4
Checking for the Correct Fuse	1-5
Getting Power to the Instrument	1-6
operating Environment	1-6
Ventilation	1-6
Loading the Operating System	1-7
Installing the Operating System Disc	1-8
Line Switch	1-9
Intensity Control	1-9
Power-up Self-Test	1-10
Summary	1-11

Chapter 2:

Getting to Know the Front Panel

Introduction	2-1
Front Panel Organization	2-1
Cursor	2-2
Keypad	2-3
Roll	2-4
Menu	2-5
Display	2-6
Disk Drive	2-7
summary	2-7

Chapter 3:	How Do I Use the Front Panel?	
	Introduction	3-1
	Menu Field Conventions	3-2
	Your First Step	33
	Returning to the System Configuration Menu	3-4
	Exploring the System Configuration Menu	35
	Closing Pop-up Menus	3-6
	Summary	37

Chapter 4:	Learning the Basic Menu8	
	Introduction	4-1
	<i>Selector</i> Pop-up Menu	4-1
	Switching Between Analyzers	4-1
	Assigning Pods	4-3
	Alpha Entry Pop-up Menu	4-4
	Changing Alpha Entries	47
	Numeric Entry Menus	4-9
	Assignment/Specification Menus	4-13
	Assigning Bits to Pods	4-13
	Specifying Patterns	4-15
	Specifying Edges	416
	Summary	4-18

Chapter 5:	Using the Timing Analyzer	
	Introduction	5-1
	Problem Solving with the Timing Analyzer	5-2
	What Am I Going to Measure?	52
	How Do I Configure the Logic Analyzer?	5-3
	Connecting the Probes	5-5
	Activity Indicators	s-5
	Configuring the Timing Analyzer	5-6
	Specifying a Trigger Condition	5-8
	Acquiring the Data	5-9
	The Tii Waveforms Menu	5-10
	The X and O	5-10
	The Vertical Dotted Line	5-11
	Configuring the Display	5-12

Display Resolution	5-12
Making the Measurement	5-13
Finding the Answer	5-14
summary	5-15

Chapter 6:

Using the State Analyzer

Introduction	6-1
Problem Solving with the State Analyzer	6-2
What Am I Going to Measure?	6-2
How Do I Configure the Logic Analyzer?	6-4
Connecting the Probes	6-6
Activity Indicators	6-6
Configuring the State Analyzer	6-7
Specifying the J Clock	6-9
Specifying a Trigger Condition	6-10
Acquiring the Data	6-12
The State Listing	6-13
Finding the Answer	6-14
Summary	6-16

Chapter 7:

Using the Timing/State Analyzer

Introduction	7-1
Problem Solving with the Timing/State Analyzer	7-2
What Am I Going to Measure?	7-2
How Do I Configure the Logic Analyzer?	7-3
Configuring the State Analyzer	7-4
Connecting the Probes	7-5
Acquiring the Data	7-5
Finding the Problem	7-6
What Additional Measurements Must I Make?	7-7
How Do I Re-configure the Logic Analyzer?	7-g
Connecting the Timing Analyzer Probes	7-8
Configuring the Timing Analyzer	7-9
Setting the Timing Analyzer Trigger	7-10
Time Correlating the Data	7-11
Re-acquiring the Data	7-12
Mixed Mode Display	7-12
Interpreting the Display	7-13
Overlapping Timing Waveforms	7-14

Finding the Answer	7-15
Summary	7-16

Chapter 8:	Making Hardcopy Prints	
	Introduction	8-1
	Hooking Up Your Printer	8-1
	Setting RS-232C for HP Printers	8-2
	Setting RS-232C for Your Non-HP Printer	8-3
	Setting HP-IB for HP Printers	8-4
	Starting the Printout	8-5
	Print screen	8-5
	Print All	8-6
	What Happens during a Printout?	s-6
	Summary	8-7

Chapter 9:	What's Next?	
-------------------	---------------------	--

Appendix A:	Logic Analyzer Turn-on Check List	
--------------------	--	--

Appendix B:	Loading Demo Files from the Disk	
--------------------	---	--

Introduction

About this book. . .

Welcome to the new generation of **HP** logic **analyzers**. The HP **1650B/51B** logic **analyzers** have been **designed** to be the easiest to use logic **analyzers** ever. In addition to being easy to use, these logic **analyzers** make a **significant** contribution to digital measurement **technology**.

That's why we'd like you to invest your time going through this ***Getting Started manual***. Whether you're a novice logic analyzer user or just new to these particular models, this book will give you a working **knowledge** of the HP **1650B/51B** so that you can start using it to solve your measurement problems. It **covers**:

- front panel **organization**;
- how to operate the front **panel**;
- **learning** the basic **menus**;
- **how to set up the analyzer**;
- how to make **basic measurements**.

To make the book easier to use, we have put the names of **keys** (FORMAT, SELECT etc.) in bold type. And we have highlighted actions (rotate the knob, press the **DISPLAY**) in color.

If you are an experienced HP logic **analyzer** user but new to this family of logic **analyzers**, you may feel like going directly to the reference manual. We'd like you to reconsider and read chapters 1 through 4 first. These chapters will **only** take a few **minutes** and you will **find** the user interface of the **HP 1650B/51B** very friendly **and** easy to learn.

Don't **worry...we** didn't **try** to cover every feature and function of the **HP 1650B/51B** logic analyzer **in** this manual. That's the job of your ***HP 1650B/51B Front-Panel*** manual.

If you're new to logic **analysis...or** just **need** a refresher, we think you'll **find** ***Feeling Comfortable With Logic Analyzers*** valuable reading. It will help you sort out any confusion you may have about their application and show you how to get the most out of your new logic analyzer.

Introducing the HP1650B/HP 1651B

What Are the HP 1650B and HP 1651B?

The HP 1650B/51B logic analyzers are new general-purpose logic analyzers with improved features to accommodate next-generation design tasks. They are basically the same as their predecessors the HP 1650A and HP 1651A, but now have State Compare, State Waveform, and State Chart modes. They both have HP-IB capabilities in addition to RS-232C. Both the 80-channel HP 1650B and the 32-channel HP 1651B logic analyzers are capable of 100 MHz timing analysis. The HP 1651B is capable of 25 MHz state analysis while the HP 1650B is capable of 35 MHz state analysis on all channels. The HP 1651B, while only having 32 channels, has basically the same features as the HP 1650B. That's why you have the same manual set regardless of whether you have an HP 1650B or HP 1651B.

The key features of the HP 1650B and HP 1651B are:

- Transitional or glitch timing modes
- Simultaneous state/state or state/timing modes
- 1k-deep memory on all channels
- Glitch detection on all channels
- Maker measurements
- Pattern, edge, and glitch triggering
- Overlappii of timingwaveforms
- Eight sequence levels
- Eight pattern recognizers
- One range recognizer
- Small lightweight probing
- Time and number of states tagging
- Pre-store
- State Compare
- State Waveform
- State Chart

Not all of these features will be covered in this Getting Started manual. However, you can find the details of these and all the features of the HP 1650B/1651B in the HP 1650B/HP 1651B Reference manual.

Getting Ready to Operate

If you have just unpacked your new HP 1650B/51B logic analyzer, please take a few minutes to completely read this chapter. It tells you how to prepare your Logic analyzer for applying power and turning it on. If you are learning how to use the logic analyzer and it is already turned on, start with with chapter 2 "Getting to Know the Front Panel".

Initial Inspection

Inspect the shipping container for damage. If the shipping container or packaging materials are damaged, you should keep them until the contents of the shipment have been checked for completeness and the instrument has been checked mechanically and electrically.

If the contents of the shipping container have been damaged or the instrument does not operate properly, refer to the service manual.


Accessories

In addition to checking the instrument for damage, you should also check to see that the accessories supplied with it are complete. Accessories can sometimes be lost in transit when the shipping container is damaged.

The *Front-Panel Reference manual* lists all the accessories for the HP 1650B/51B logic analyzers. If any of these items are missing contact your nearest Hewlett-Packard office.

Removing Yellow Shipping Disc

Your logic analyzer is shipped with a protective yellow shipping disk in the disk drive. Before you can insert the operating system disk you must remove the yellow shipping disk. Press the disk eject button as shown in the figure. The yellow shipping disk will pop out part way so you can pull it out of the disk drive.

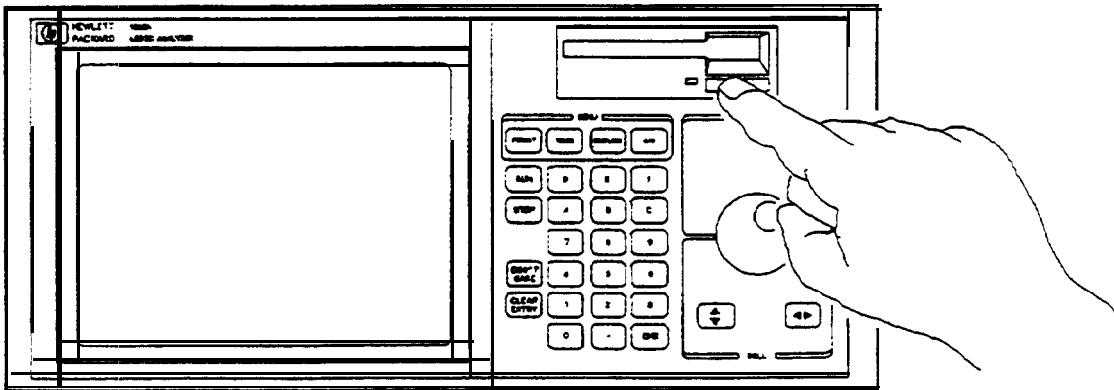


01650E01

Selecting the line Voltage

The line voltage selector has been factory set to the line voltage used in your **country**. It is a good idea to check the setting of the line voltage selector so you can become **familiar** with what it looks like. If the **setting needs to be changed, follow the procedure in the next paragraph.**

CAUTION 


You can damage the logic **analyzer** if the module is not set to the **correct position.**

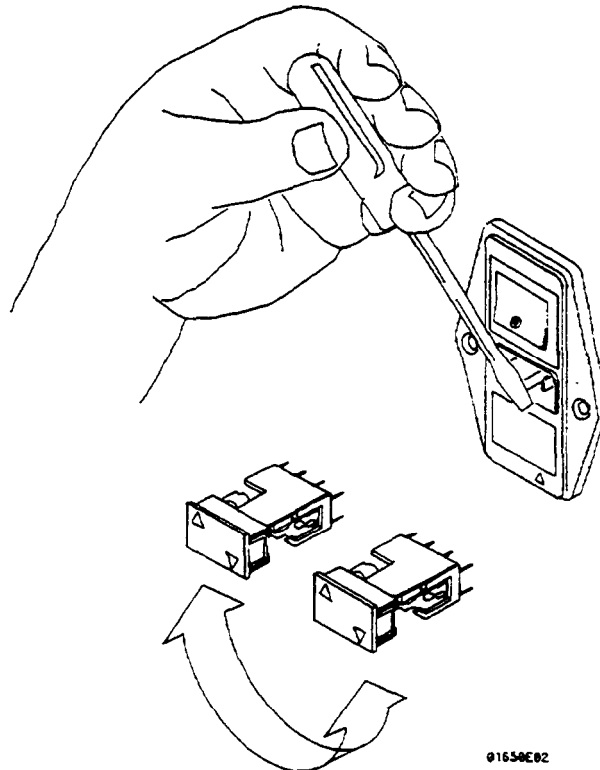

You change the line voltage setting by pulling the fuse module out and **reinserting** it with the **proper** arrows aligned. To remove the **module, carefully** pry at the top center of the module (as shown) until you can grasp it and pull it out by hand.

Checking for the Correct Fuse

If you need to check for the correct fuses, remove the fuse module and look at the amperage and voltage of each fuse. The following figure will help you locate the 115 V and 230 V fuses. To remove the fuse module, carefully pry at the top center of the module until you can grasp it and pull it out by hand. (Refer to "Selecting the Line Voltage" on the previous page.)

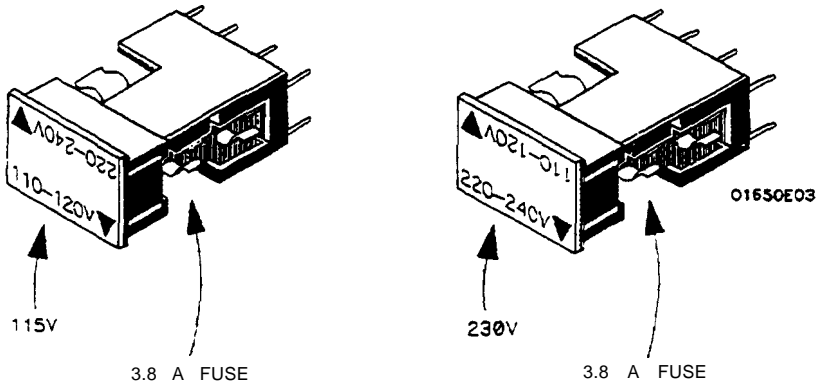

Getting Power to the Instrument

The HP **1650B/51B** comes with a **3-wire** power cable. When you **connect** the **cable** to **an appropriate** AC power receptacle, a ground is provided for the **instrument** cabinet. The type of power cable you **receive** with the instrument depends on your **country**.

WARNING 

To avoid possible shock hazard, you must connect the instrument to a properly grounded **3-wire** receptacle.

Operating Environment

You may operate your logic **analyzer** in a normal lab or office **environment** without any additional considerations. But don't block its **ventilation**. If you intend to use it in another type of **environment**, you **must not exceed certain limits**. **You can find these limits in the HP 1650B/HP 1651B Front-Panel Reference manual**.

Ventilation

You must provide an unrestricted airflow for the fan and ventilation openings in the rear of the logic **analyzer**. However, you may stack the logic analyzer under, over, or in-between other instruments as long as **the** surfaces of the other instruments aren't needed for their ventilation.

Loading the Operating System

Before you can operate the logic analyzer, it must transfer its operating system from a disk to its memory. This is called "loading the operating system" or "booting."

The logic analyzer operating system is a set of instructions that control the operation of the instrument. The operating system resides on a 3.5-inch flexible disk. You received two identical operating system disks. You should mark one of them Master and store it in a safe place. Mark the other one Work and use only the work copy. This will provide you with a back-up in case your work copy becomes corrupt.


CAUTION



To prevent damage to your operating system disk, DO NOT remove the disk from the disk drive while it is running. Only remove it after the indicator light has gone out

Installing the Operating System Disc


To load the **logic analyzer's** operating system, you **must** install the disk as shown below **before** you **turn on** the power. When the disk snaps into place, **the** disk eject button **will** pop out. Now you can turn on the logic analyzer.

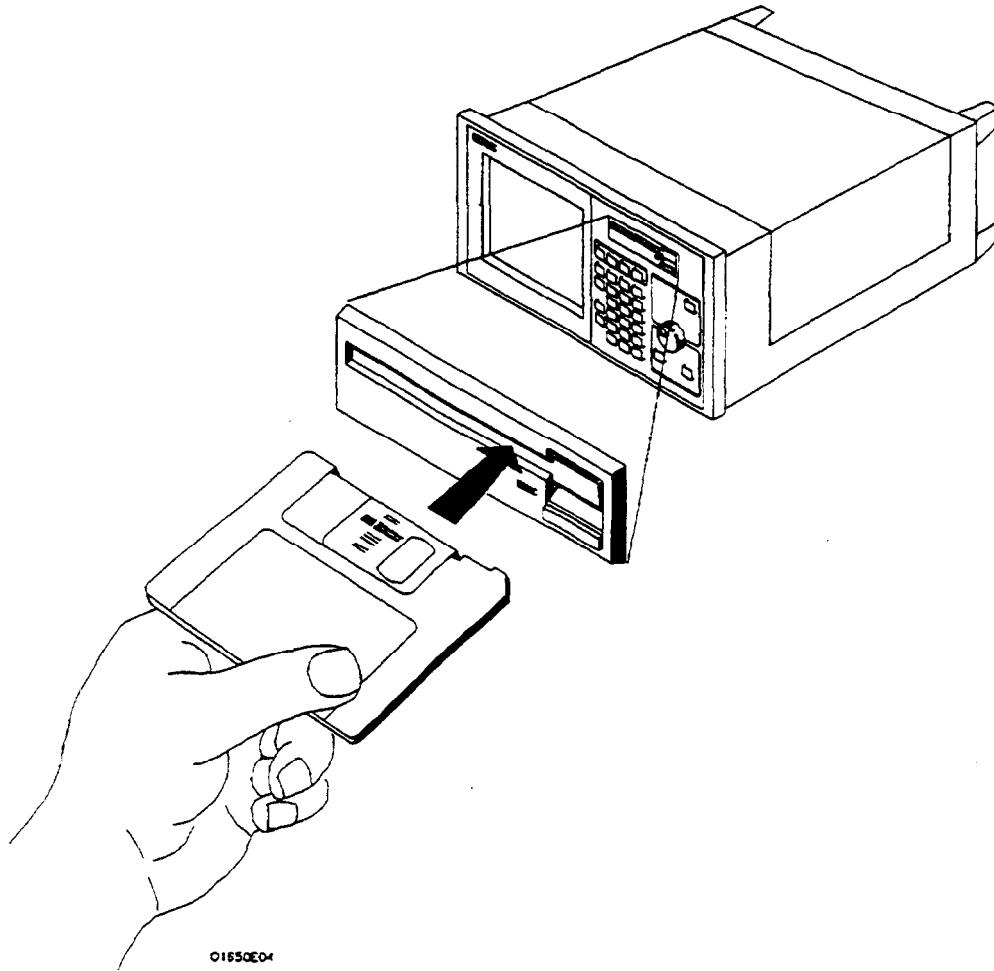

The logic analyzer runs a series of self-tests and loads the operating system before it is ready to be operated.


Line Switch

The line switch is on the rear panel. You turn on the logic analyzer by pressing the 1 on the rocker switch. Make sure the operating system disk is in the disk drive before you turn it on. If you forget the disk, don't worry, you won't harm anything. You will merely have to repeat the turn-on procedure with the disk in the drive.

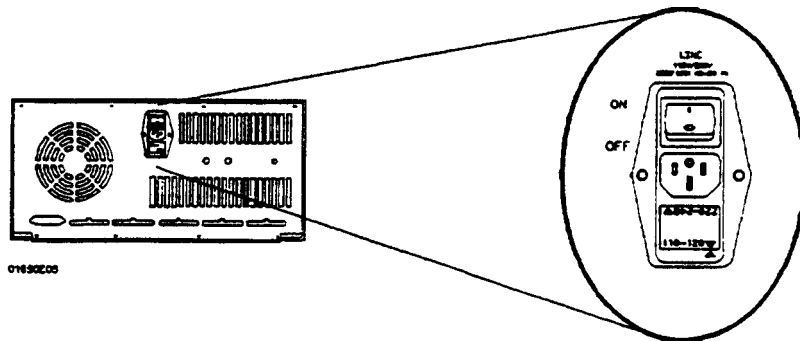

Intensity Control


Once you have turned on the instrument, you may want to set the display intensity to a different level that's more comfortable for you. You do this by turning the **INTENSITY control** on the rear panel.

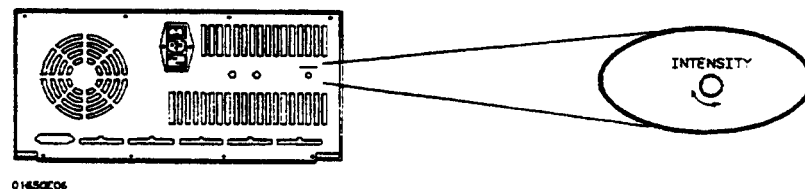

Power-up Self-Test

When you turn on the logic analyzer, it performs a series of self-tests. When it has successfully completed these tests, it loads the operating system into memory from the disk

When the logic analyzer has completely loaded the operating system it displays the System Configuration menu as shown below.

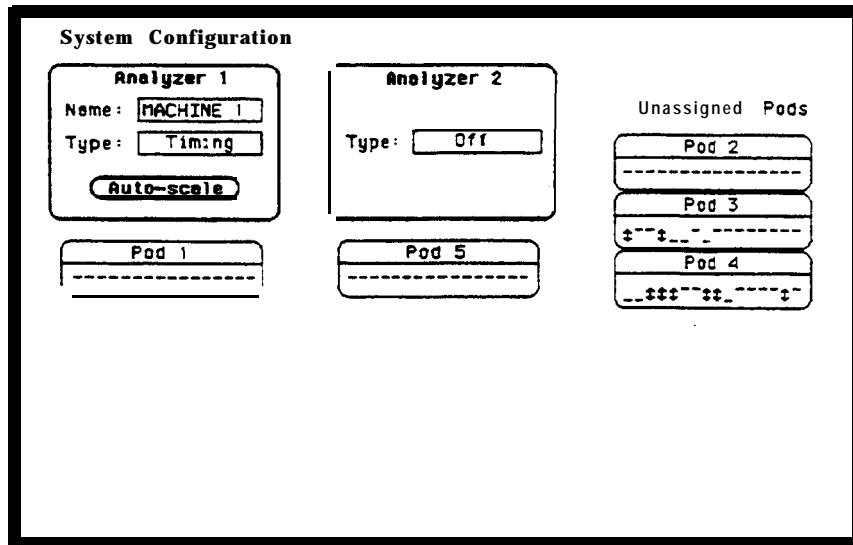

Note



This is the HP 1650B System Format Specification menu. If you have an HP 1651B, the only difference is pod 1 will be assigned to analyzer 1 and pod 2 will be assigned to analyzer 2. There won't be any pods in the UNASSIGNED area of the display.

Summary

Now that you have unpacked, inspected, and begun operating the logic analyzer, the next step will depend on your needs. If you are a first-time logic analyzer user who wanted to get the instrument running before reading *Feeling Comfortable with Logic Analyzers* you should read it now. If you are familiar with logic analysis, read either the rest of this *Getting Started Guide* or the *HP 1650B/HP 1651B Front-Panel Reference Manual*.

In a task format this *Getting Started Guide* teaches you the basics of how to operate the front panel and configure it for basic measurements.

The *HP 1650B/HP 1651B Front-Panel Reference* manual describes all the front-panel and programming functions of the logic analyzers. The *HP 1650B/HP 1651B Programming Reference* manual describes the programming commands and conventions for the logic analyzers. Once you feel comfortable with the basic operation of the front panel, use this book.

Getting to Know the Front Panel


Introduction

The HP 1650B/51B logic analyzers have been designed to be very easy to use. The controls are located logically by function so you can learn how to use them quickly and easily.


This chapter breaks down the front panel into these functional areas and gives you an overview of each area.

Front Panel Organization

The functional areas of the front panel are: display, MENU, keypad, CURSOR, ROLL and disk drive.

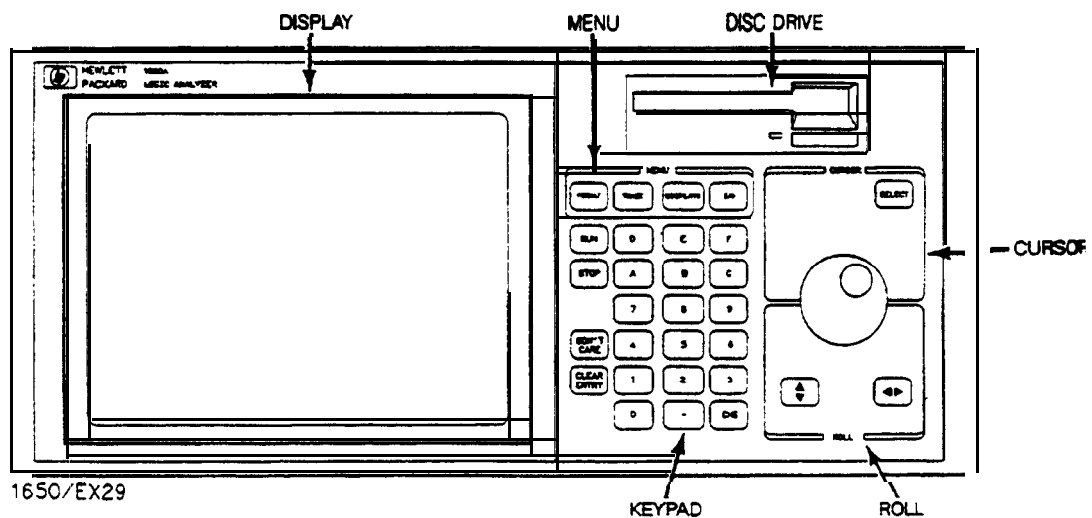


Cursor The CURSOR is a movable indicator on the display that allows you to access desired fields in **each menu**. It changes the field where it resides from the normal white **background** to the dark **background** (inverse video). The KNOB moves the cursor to the field (function) you wish to use. You **activate** the field (**function**) by pressing the SELECT key.

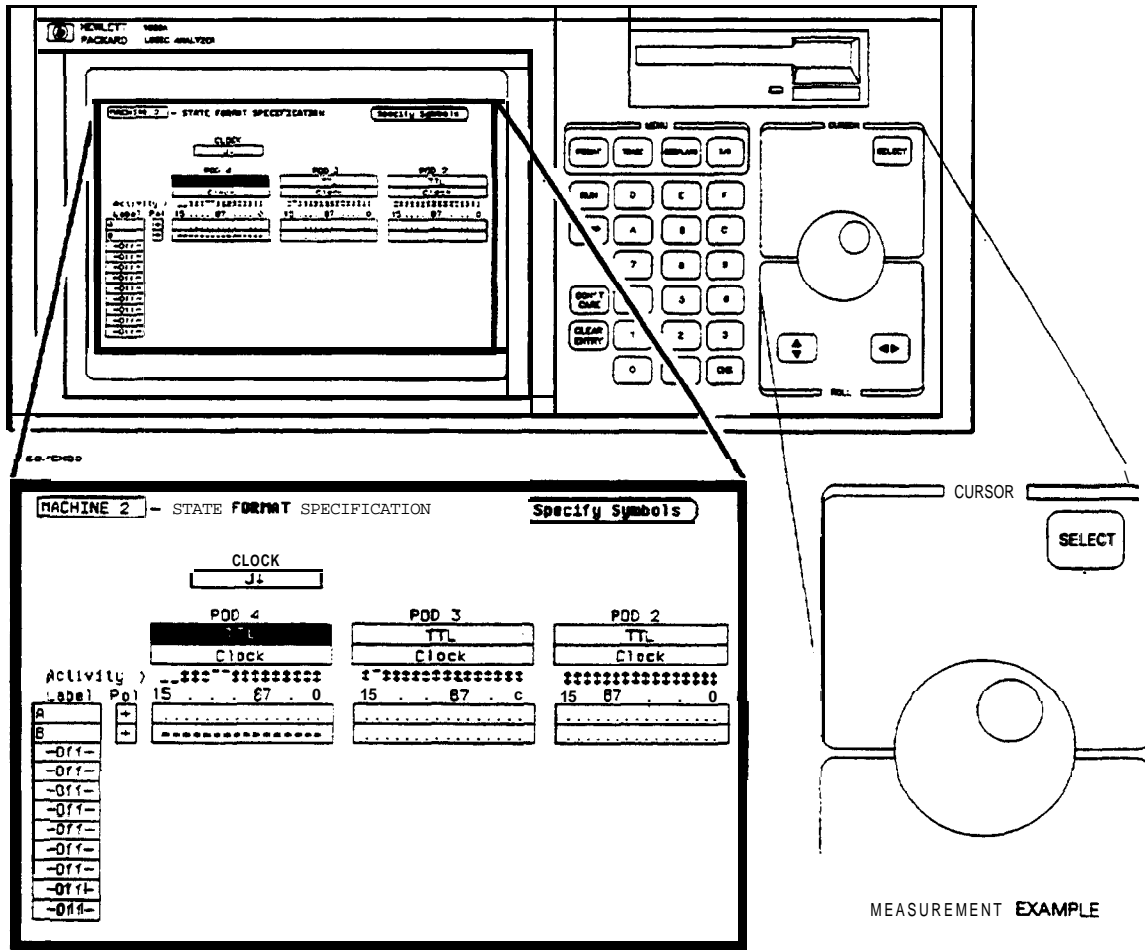



MENU EXAMPLE

MEASUREMENT EXAMPLE


Keypad The keypad allows you to start and stop data acquisition as well as enter alphanumeric data. Also in the keypad area are the DON'T CARE and CLEAR ENTRY keys.

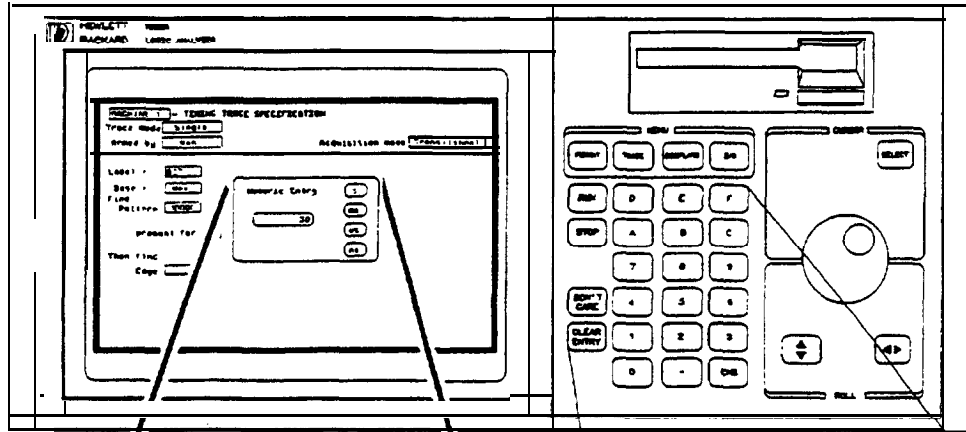


1650/EX32

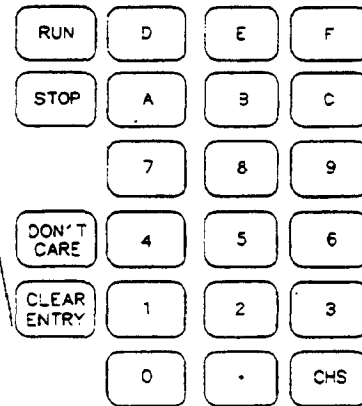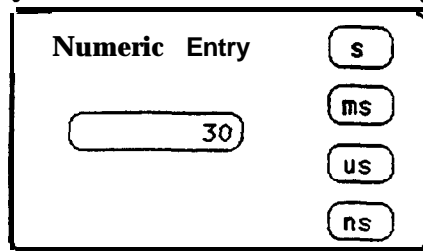

Menu The MENU area contains keys that give you access to the four major menus of the logic analyzer. You use this area to:

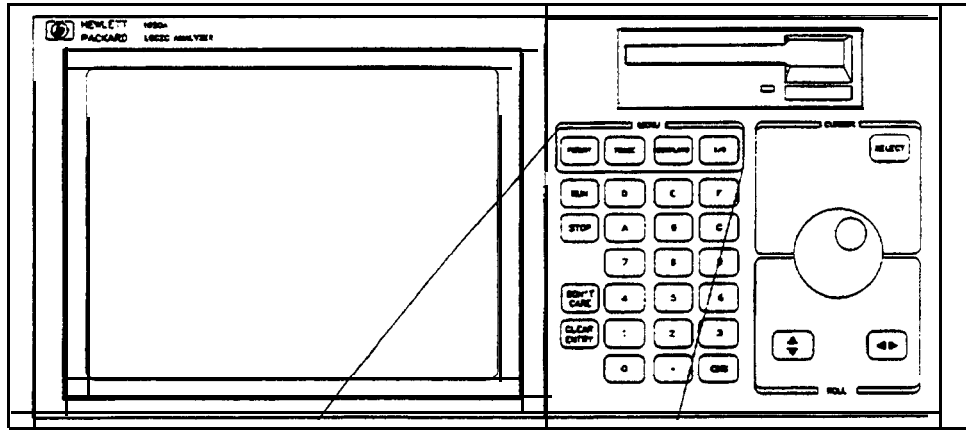

1650/EX31

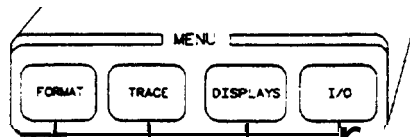


- Access disc drive functions and set up the analyzer for use with a printer or controller.

Choose how the acquired data will be displayed

- Specify how and when each analyzer type will acquire data for your measurement.

Select the timing/state format specification menus where you assign names to channels

Display The display shows you the **menus** for configuring the logic analyzer and the results of your measurements.

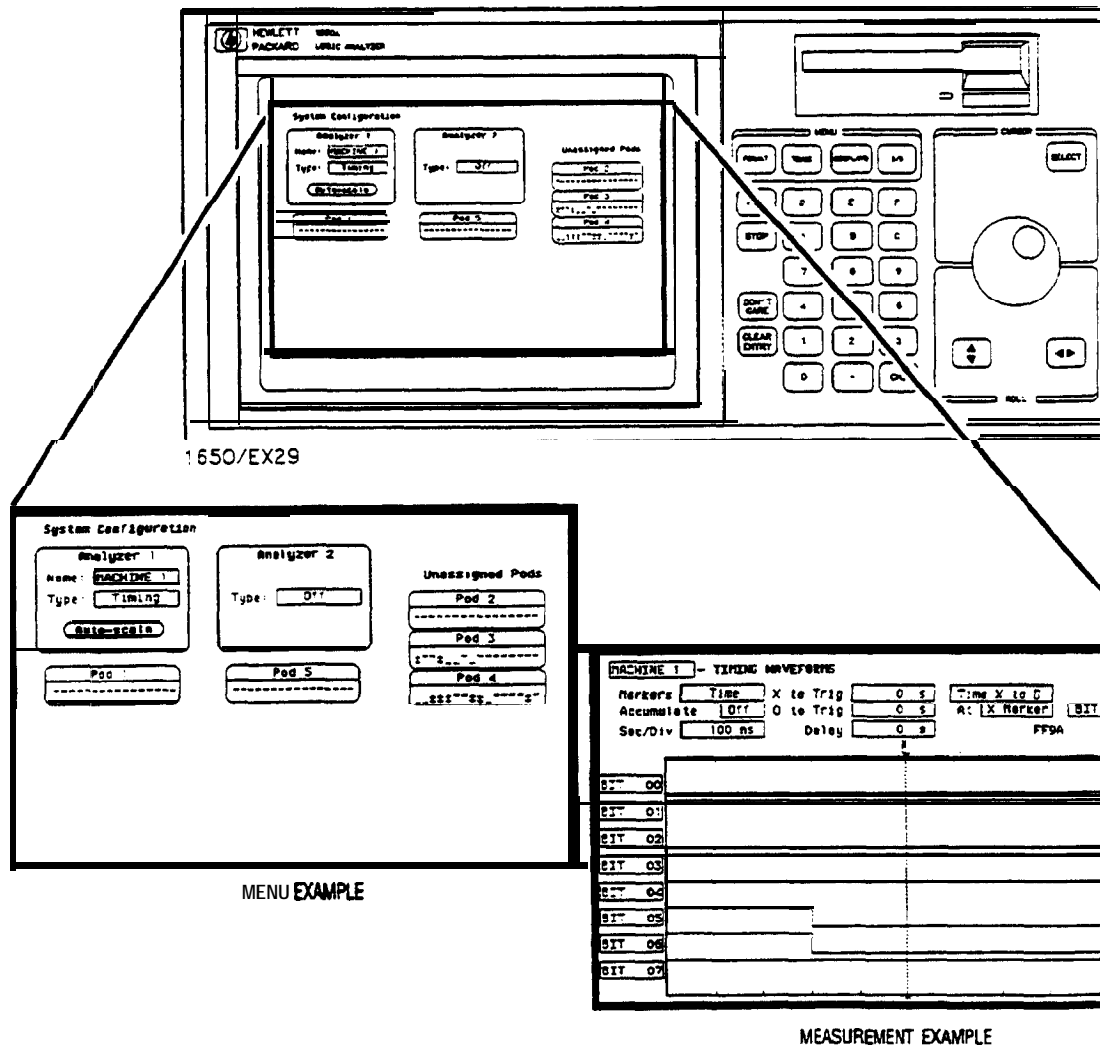

Disk Drive The logic analyzer uses the disk drive every time you **turn** on the logic analyzer to load its operating system. The disk drive uses **3.5-inch flexible disks**. You can also use the disk drive to store instrument configurations, acquired data, and inverse assemblers for later use. Complete details on the disk drive and its functions can be found in the *li?' 1650B/HP 1651B Front-Panel Reference manual*.

Summary

Now that you are acquainted with the front panel organization, you **will** be able to decide where you want to go **next**. If you are just **starting** to learn logic analysis, you should read this entire manual. If you are **experienced in** logic analysis, you should **continue** to read **chapters 3 and 4** to become more **familiar with** the operation of **the front panel** before you **turn** to the reference **manual**. **These** chapters will show you how easy the HP **1650B/51B** logic **analyzers** are to operate.

How Do I Use the Front Panel?

Introduction

In this chapter you will learn how easy the HP 1650B/51B logic analyzer front panel controls are to use. You will also learn the front panel by following self-paced exercises.

This chapter starts you off in the System Configuration menu, the same place the logic analyzer starts after you turn it on. You will learn how easy it is to get in and out of this menu. You will also learn what the shapes of the menu fields mean

Don't be concerned about not seeing measurement examples in this chapter. You will see them in chapters 5 through 8.


Menu Field Conventions

Before starting to work with the menus, you need to know the two menu field conventions. This allows you to quickly recognize what type of action will occur when you select a field.

There are two shapes that you should become familiar with: rectangles with square corners and rectangles with rounded corners.


When you select a field with square corners, it pops up and lists two or more items. You must select a single item.

Fields with rounded corners will either execute the function immediately or pop up with a list of multiple items that you must specify.

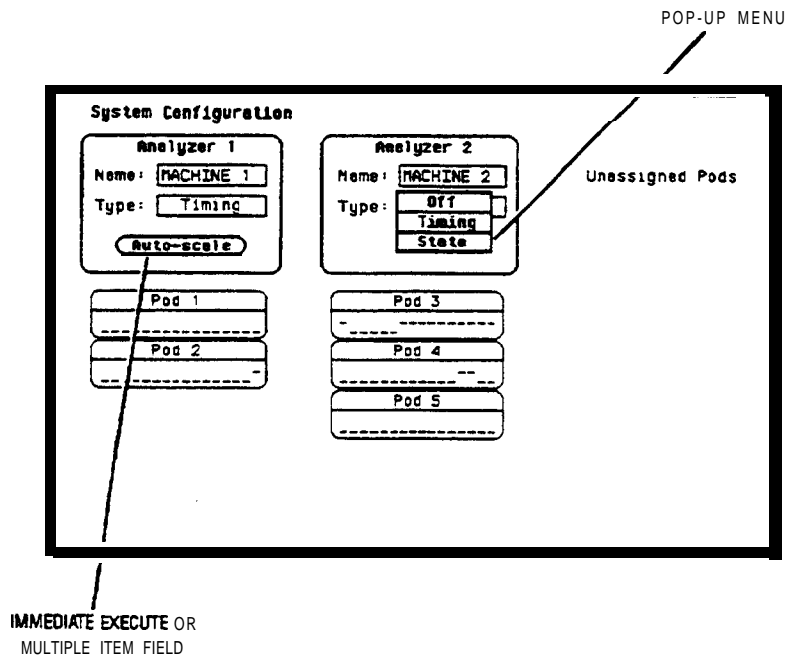

Your First Step

When you turn on the logic analyzer and the operating system has finished loading, you will see the System Configuration menu. Notice the cursor is in one of the fields in this menu. Operating the HP 1650B/51B front panel is like leaning to drive a car.

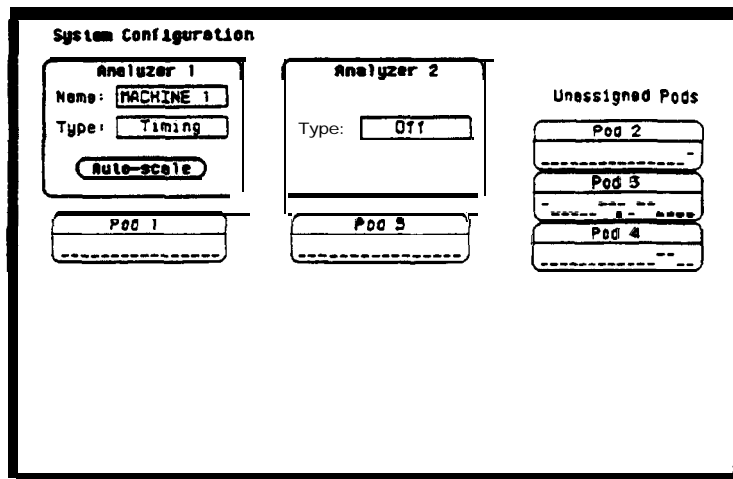

To “drive” around the menu, turn the KNOB and watch the cursor move from field to field. Most of the logic analyzer operation is accomplished by placing the cursor on the field you want to interact with and pressing the SELECT key. Depending on the field type (immediate execute or pop-up) pressing SELECT will either execute a function or open a pop-up menu.


Note 

This is the ZIP 1650B System Format Specification menu. If you have an HP 1651B, the only difference is pod 1 will be assigned to analyzer 1 and pod 2 will be assigned to analyzer 2. There won't be any pods in the UNASSIGNED area of the display.

Returning to the System Configuration Menu

When you leave the System Configuration menu, you can return to it at anytime by following these steps

1. Press either the FORMAT, TRACE, or DISPLAY key. You now see a new menu. All three of these menus have a field in the upper left corner. This field will display either MACHINE 1 or MACHINE 2 depending on how the logic analyzer was configured.
2. Place the cursor on this field and press SELECT. You will see the following pop-up menu.
3. Place the cursor on System and press SELECT. You will be returned to the System Configuration menu

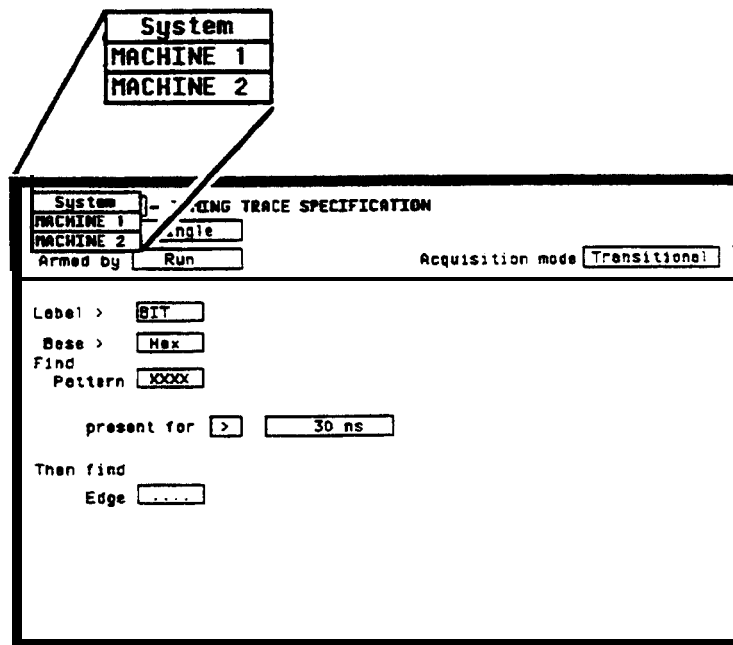

Exploring the System Configuration Menu

Now is a good time to explore the System Configuration menu by driving the cursor around and pressing SELECT. Don't worry, you can't hurt anything because no matter what field you select you will have an easy way out.

For example, select the Name: MACHINE 1 field, and you will see a pop-up that you can use to name analyzer number 1. In this pop-up menu you will see a field named Done that lets you get out of this menu and back to the System Configuration menu where you started.

If you select Auto-scale, the logic analyzer will display a pop-up with the choices of Cancel and Continue. The Cancel allows you to change your mind before the auto-scale is executed. This is handy because auto-scale will change your previous configurations .

If you select Continue, the logic analyzer will display the TIMING WAVEFORMS menu. However, if there is no signal activity at the probes, the Waveforms menu will not display data and the label to the left of the waveform area will be -off-.

To get back to the System Configuration menu after executing Auto-scale:


1. Place the cursor on the field in the upper left corner and press SELECT.
2. Place the cursor on System in the pop-up and press SELECT. You will now be back in the System Configuration menu.

Closing Pop-up Menus

In previous exercises, you closed the Alpha Entry pop-up by using the Done field. But, what if there is no Done in the other fields? Fields that don't have choices like Done, Cancel, or Exit will close automatically when you make your selection. For example, you have used this type of pop-up to get back to the System Configuration menu.

To see another example of a pop-up that automatically doses, follow these steps:

1. Rotate the KNOB until the cursor is on the Off field in the ANALYZER 2 field, then press SELECT. You will now see the following pop-up:

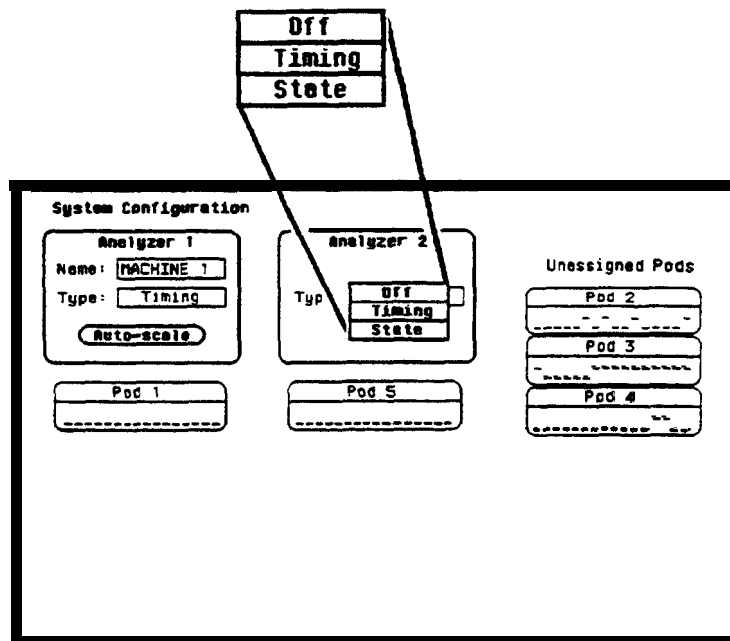

2. Place the cursor on State and press Select.

The pop-up menu will automatically dose, analyzer 2 is now on and the type will be State.

Summary

In this chapter you learned what menu the logic analyzer displays once you have turned it on and where you will usually start configuring the logic analyzer once you are ready to make measurements.

The next chapter will teach you the most common types of pop-up menus, which will help you progress towards making measurements as explained in chapters 5 through 7.

Learning the Basic Menus

Introduction

in this chapter you **will** learn the most common **pop-up** menu types by doing some basic exercises. The pop-up menu types you will **learn** in **this** chapter **are**:

- Selector
- **Alpha Entry**
- **Numeric Entry**
- **Assignment/Specification**

Selector Pop-up Menu


In the selector type of pop-up **menu** you do what the name implies, make a **selection** from **two** or more **options**. The best way to **introduce** you to a **selector** type of menu is to **have** you work **with** one right away.

Switching Between Analyzers

You **will** use a selector type of **pop-up** menu to switch between analyzers or get back to the System **Configuration** menu- You can **switch analyzers in the** FORMAT, TRACE **and** DISPLAY **menus**, without having to go back to the System Configuration menu. This is done easily by following these steps:

1. Press the TRACE key. You will now be **in** either the TIMING **TRACE** or **STATE** TRACE **SPECIFICATION** menu depending on **what** you did last in the System **Configuration** menu.

- Place the cursor in the field in the upper left corner of the menu and press **SELECT**. A pop-up menu will appear displaying System and the current analyzer names (default names are **MACHINE 1** and **MACHINE 2**). The cursor will be on the current analyzer.

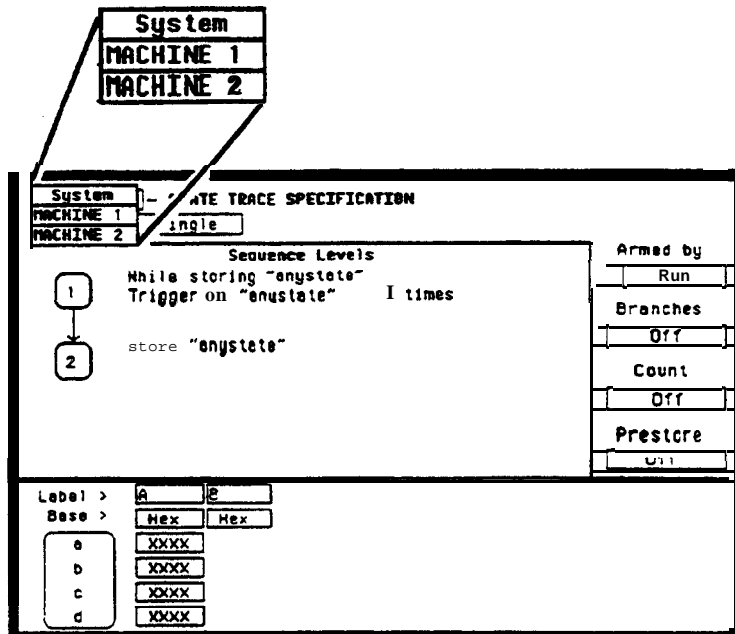


- Move the cursor to the other machine (analyzer) and press **SELECT**. The pop-up will close and you will see the corresponding menu of the other analyzer on the display.

Assigning Pods

Another selector menu type you will use is assigning pods to the analyzers. To assign pods:

- 1 Get back to the System Configuration menu (refer to “Returning to the System Configuration Menu” in chapter 3 if you need a reminder).
- 2 Place the cursor on one of the pod fields on the **right** side of the display and press **SELECT**. You will see the following menu:

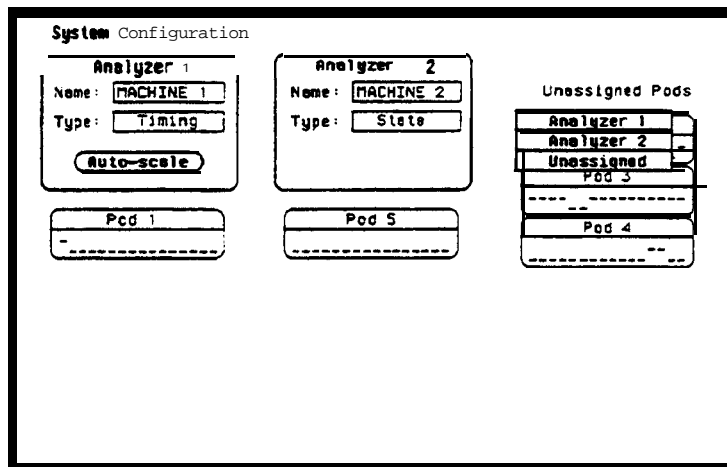

3. Place the cursor on Analyzer 2 and press **SELECT**. The pop-up closes and your desired pod is now assigned to analyzer 2

Alpha Entry Pop-up Menu

You can give specific names to several things. These names can represent your measurement specifically.


The two major examples of items that can be named are:

- Bothana@crs
- @B@/M@


To learn how **this** type of pop-up works, you'll name analyzer 1 LEARN. However, LEARN will be misspelled when you **finish** entering it. **Don't worry**, this is **intentional**. You will then be shown how to correct it.

1. Get back to the System Configuration menu refer to "Returning to the System Configuration Menu" in chapter 3 if you need a reminder).
2. Rotate the KNOB until the cursor is over MACHINE 1 and press **SELECT**.

You will now see a pop-up window in the System Configuration menu as shown in the example.

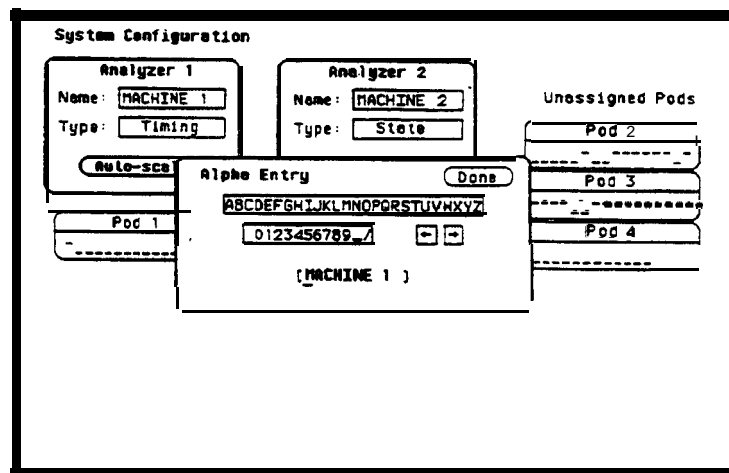

3. Rotate the KNOB and you will see how the cursor moves within the pop-up.

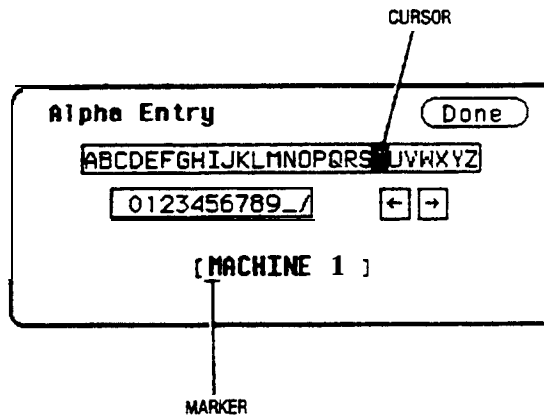

4. Now that you are ready to name **analyzer 1**, move the cursor so that it is on the L and press **SELECT**.

In the bottom of the **pop-up**, you will see an L in the far left corner of the bottom box. Also notice the under-score marker in the bottom box is now under the A of MACHINE. The under-score marker tells you in what space in the box your next selection will be placed.


5. Rotate the KNOB again until you have placed the cursor over the E, then press **SELECT**.

Note 

You can also make direct keypad entries. Your selection will be placed where the under-score marker is in the box.

6. Repeat step 5 three more times selecting A, R, and M respectively.


You should now see **LEARMNE 1** in the bottom box. Since this is not the name you wanted, change the name.

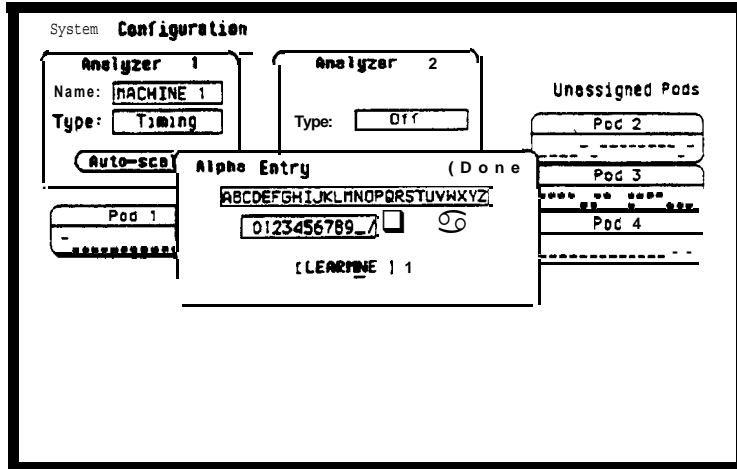

Changing Alpha Entries

To make changes or **corrections** in the Alpha Entry field, place the under-score marker **under** the character you want to change.

To move the under-score marker **to the** left, place the cursor over the **left arrow** and **press SELECT once** for each backspace.

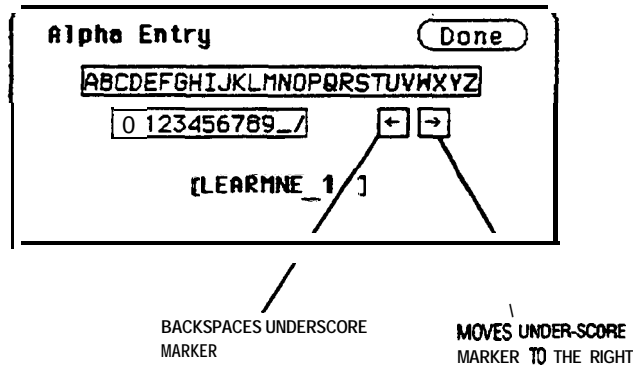


To move the under-score marker **to the right**, you **either** place the cursor on a desired character and press SELECT, or place it on the right arrow and press **SELECT**.

You **can** also use the ROLL **Keys** and the KNOB to move the underscore marker. To use **this alternate method**:

1. Press the **left/right** ROLL key.
2. Rotate the KNOB to place the under-score marker **under** the desired character.
3. Press the left/right ROLL **key again** to **turn** off the ROLL function

If you want to **erase** the entire entry and place the **underscore** marker at the **beginning** of the name box, press the **CLEAR ENTRY** key on the front panel.

If you want to replace a **character** with a space, place the **underscore** marker under that character and press the **DONT CARE** key on the front panel.

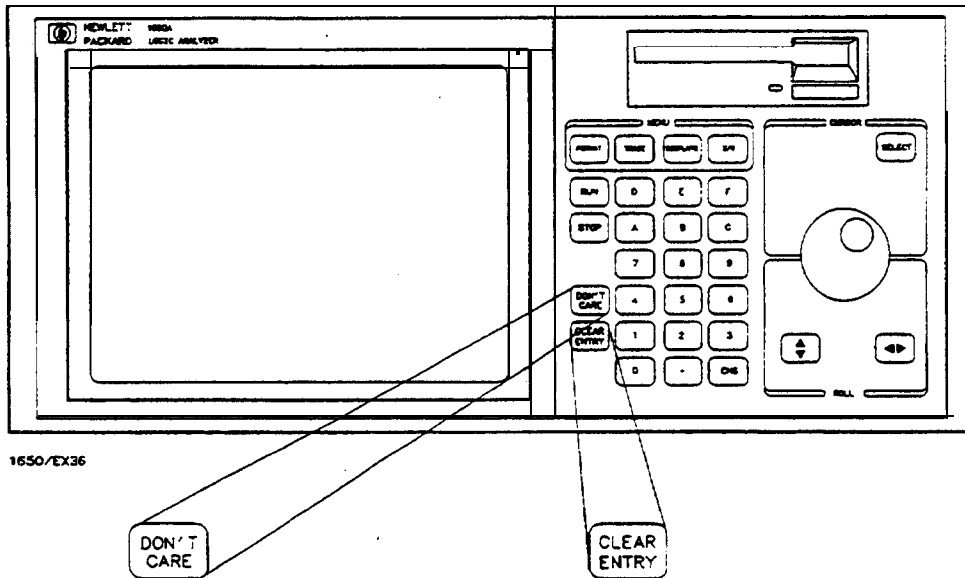

1650/EX36

Now that you have entered and edited a name, you will know how to use the Alpha Entry pop-up menu in other logic analyzer menus where it appears.

Numeric Entry Menus

There are many pop-up menus in which you enter numeric data. The two major types are:


-  (i.e. )
- Numeric entry with variable units (i.e. ms, μ s, etc.)

There are several numeric entry menus in which you only enter the value, and the units are fixed. One such type of numeric entry pop-up is the POD **Threshold pop-up menu**.


Besides being able to set the pod thresholds to either of the preset thresholds (TTL or ECL), you can set the thresholds to a specific voltage from -9.9 V to +9.9 V.

To set pod thresholds to a specific voltage, follow these steps:

1. Select either the **TIMING** or STATE FORMAT SPECIFICATION menu by pressing the **FORMAT** key. It doesn't matter whether you are in the **TIMING** or STATE FORMAT SPECIFICATION menu.
2. Rotate the KNOB to place the cursor in the TTL field of any pod displayed and press SELECT. You will now see a pop-up with the choices, **TTL**, **ECL**, and User defined.

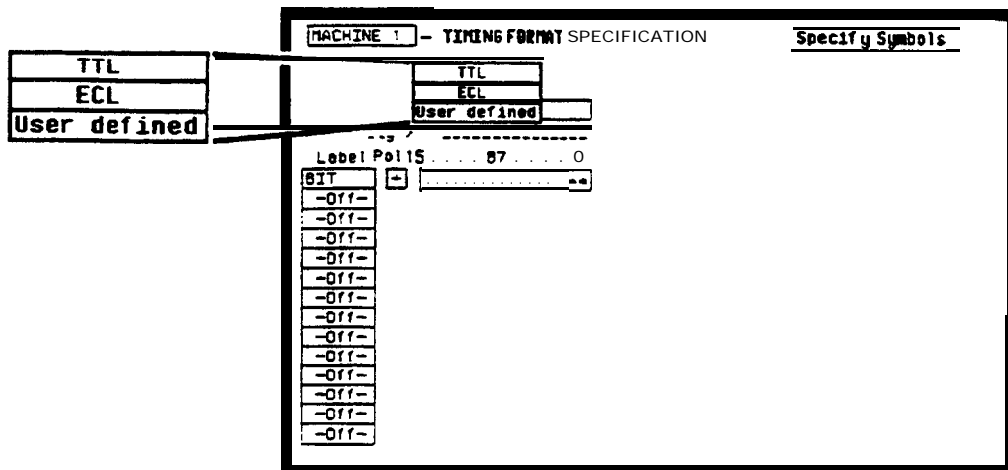

- Place the cursor on User **Defined** and press SELECT. Another pop-up menu will appear as shown.

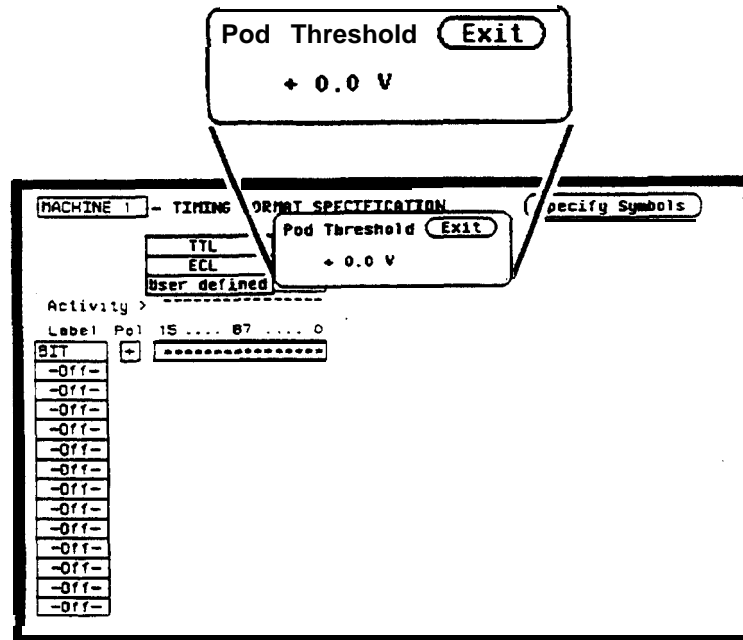


You can enter your desired threshold with either of two methods when the pod threshold **pop-up** is **open**. The first method is to rotate the KNOB until your desired threshold is displayed- Rotating the KNOB increments or decrements the value in small **increments**.

The **second** method is to use the keypad, which allows you to change large values quickly. With the keypad follow these simple steps to enter -5.0 V for the pod threshold:

- Enter 5.0 from the keypad. You **will** see the 0.0 V replaced with 5.0.

5. Press the **CHS** (change sign) key on the front panel. You will now see -5.0 in the pop-up.

Also notice the cursor is in the upper right corner of the pop-up over the operative Exit. When you press **SELECT**, the pop-up will close and your new threshold will be placed in the Pod field.

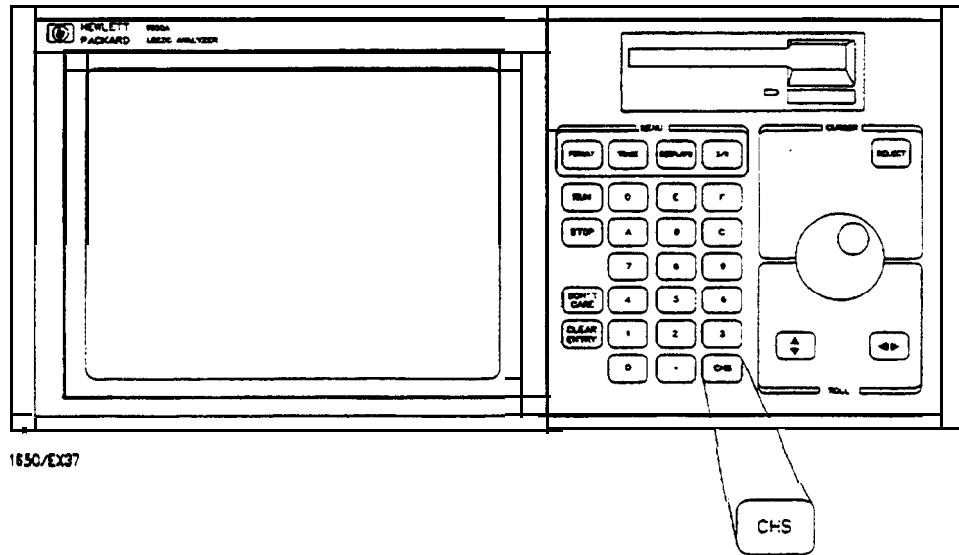


Another type of numeric entry you will use requires you to specify the units as well as the numeric value. The following steps show you how

1. Select the TIMING TRACE SPECIFICATION menu by pressing the **TRACE** key.

Note 

If the STATE TRACE SPECIFICATION menu comes up, refer to "Switching Between Analyzers" in this chapter.

2. Rotate the KNOB to **place** the cursor in the 30 ns box within the **present for > 30 ns line** and press SELECT. You **will** now see the following pop-up:

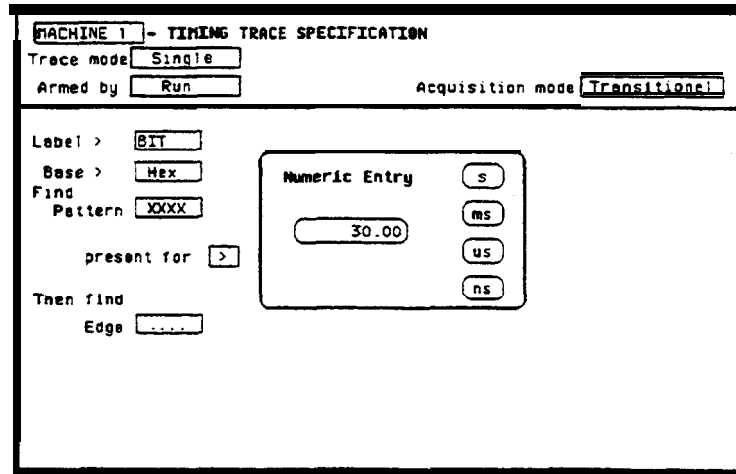


3. Enter a new value to replace 30.00 **with** the keypad. When you have entered your desired value, you can change the **units** type by **rotating** the KNOB.

Once you have selected the new value and the units, close the **pop-up** by pressing **SELECT**. **The new** value and the units will now **be** displayed in the **present for > _____** field.

2. Place the cursor on one of the bit assignment fields and press **SELECT**. You will see the following **pop-up menu**.

Note 

If you don't see any bit **assignment** fields, it merely means you don't have any pods assigned to this **analyzer**. **Either switch** analyzers or **assign a pod to the analyzer you are working with**.

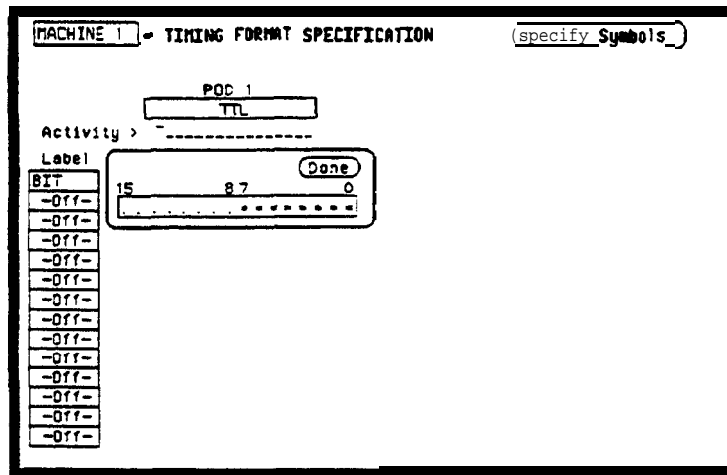

3. Rotate the KNOB to **place the** cursor on one of the asterisks or **periods** in the pop-up and press **SELECT**. You will notice how the bit assignment toggles to the opposite state of what it was when the pop-up opened.



4. You close the pop-up by placing the cursor on **Done** and pressing **SELECT**.

Specifying Patterns

The Specify **Patterns** fields appear in several menus in both the timing and state analyzers. Patterns can be **specified** in one of **several** number **bases**; however, for now we'll use hexadecimal (HEX) since it is the **default** base.

Before starting this exercise you need to know how the logic **analyzer** **knows** which pattern to ignore (doesn't care about). Whenever you see an **"X"** in this type of menu, it indicates a "don't **care**."

To specify patterns:

1. **Select** the TIMING TRACE SPECIFICATION menu
2. **Place the cursor on the Find Pattern** _____ field and press SELECT. You **will see** the **following** pop-up menu.

The screenshot shows a terminal window titled "MACHINE 1 - TIMING TRACE SPECIFICATION". The menu contains the following fields and options:

- Trace mode: Single
- Armed by: Run
- Acquisition mode: Transition
- Label > BIT
- Base > Hex
- Find Pattern: XXXX
- Specify Pattern: XXXX (pop-up)
- present for > 30 ns
- Then find Edge:

3. Type in **2, 3, 4**, and press the DON'T CARE key. You will see 234X in the pop-up. This will **be** the pattern in **hexadecimal** that you want the logic analyzer to **recognize**.
4. Close the pop-up by pressing **SELECT**.

Specifying Edges

You **specify** edges in the **TIMING TRACE SPECIFICATION** menu by following **these** steps:

1. **Press** the TRACE key. Switch to the timing **analyzer** if the STATE TRACE **SPECIFICATION** menu is displayed.
2. **Place the cursor on the Then find Edge .. field** under one of the **labels** and press **SELECT**. The following pop-up will **appear**.

MACHINE 1 - TIMING TRACE SPECIFICATION

Trace mode:

Armed by: Acquisition mode:

Label >

Base >

Find

Pattern

present for >

Then find

Edge

Specify Edge:

You will **notice 16 periods in the pop-up** menu. Each period represents an unassigned bit for each bit assigned to the **label**. **Don't** be alarmed if you have a different number of **unassigned** bits; it merely **means** the **number** of bits in your label is different than the label in this example.

Specify Edge:

↓
.....
.....
.....
.....
.....
.....
.....
.....
.....
.....
.....
.....
.....
.....
.....

3. **Place the cursor on one of the unassigned bit periods** and press **SELECT** once. You will now see **an** arrow pointing down.

Specify Edge:
 ↓.↑.

4. Move the cursor to another unassigned bit period and press **SELECT** twice. You will see an arrow pointing up.

Specify Edge:
 ↓.↑. \$. ...

5. Move the cursor to yet another unassigned bit period and press **SELECT** three times. You will see an arrow pointing both up and down.

You have just selected a positive-going (↑), negative-going (↓), and either edge (|) for your edge parameter.

6. Place the cursor on Done and press **SELECT**. The pop-up will close and you will see the following display.

MACHINE 1 - TIMING TRACE SPECIFICATION

Trace mode: Acquisition mode:

Armed by:

Label >

Base >

Find Pattern

present f o r >

Then find Edge

Note 

When you close the pop-up after specifying edges, you will see dollar signs (\$\$. .) in the Then find Edge field if the logic analyzer can't display the edges correctly. This indicates the logic analyzer can't display the data correctly in the number base you have selected.

Summary

In this chapter you **have learned** *some* of the most common **pop-up** menu types. You **will** use these pop-up menus as you set up the **logic** analyzer in the measurement example exercises in chapters 5 through 7.

If you are already **familiar** with logic **analysis** and feel you are comfortable enough with **the** HP 1650B/51B user interface, you may be ready for the HP *1650B/51B Front-Panel Reference*.

If you are not **familiar with** logic **analyzers** or logic **analysis**, you should **continue with this manual**.

Using the Timing Analyzer

Introduction

In this chapter you will learn how to use the timing analyzer by setting up the logic analyzer to make a simple measurement. We give you the measurement results as actually measured by the logic analyzer, since you may not have the same circuit available.

The exercise in this chapter is organized in a task format. The tasks are ordered in the same way you will most likely use them once you become an experienced user. The steps in this format are both numbered and lettered. The numbered steps state the step objective. The lettered steps explain how to accomplish each step objective. There is also an example of each menu after it has been properly set up.

How you use the steps depends on how much you remember from chapters 1 through 4. If you can set up each menu by just looking at the menu picture, go ahead and do so. If you need a reminder of what steps you need to perform follow the numbered steps. If you still need more information about "how," use the lettered steps.

When you have finished configuring the logic analyzer for this exercise, you can load a file from the operating system disk. This file configures the logic analyzer the same way it is configured for this exercise. It also loads the same data acquired for this exercise so you can see what it looks like on screen.

In order to learn how to configure the logic analyzer, we recommend that you follow the exercise to "Acquiring the Data" before loading the file from the disk.


You can also compare your configuration with the one on the disk by printing it (if you have a printer) or making notes before you load the file.

Problem Solving with the Timing Analyzer

In this exercise, assume you are designing a dynamic RAM memory (DRAM) controller and you must verify the timing of the row address strobe (RAS) and the column address strobe (CAS). You are using a 4116 dynamic RAM and the data book specifies that the minimum time from when LRAS is asserted (goes low) to when LCAS is no longer asserted (goes high) is 250 ns. You could use an oscilloscope but you have an HP 1650B/51B on your bench. Since the timing analyzer will do just fine when you don't need voltage parametrics, you decide to go ahead and use the logic analyzer.

What Am I Going to Measure?

After configuring the logic analyzer and hooking it up to your circuit under test, you will be measuring the time (x) from when the RAS goes low to when the CAS goes high, as shown below.

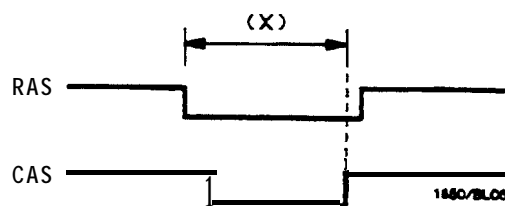


How Do I Configure the Logic Analyzer?

In order to make this timing measurement, you must configure the logic analyzer as a timing **analyzer**. By following these steps you **will** **configure Analyzer 1 as the timing analyzer**.

If you are **in** the System **Configuration** menu you are in the right place to get started and **you** can start with step 2; otherwise, start with step 1.

- Using the field in the upper left **corner** of the display, get the system **Configuration** menu on screen
 - Place the cursor on the field in the upper left corner of the display and **press** SELECT.
 - Place the cursor on **System** and press SELECT.
- In** the System **Configuration** menu, change Analyzer 1 type to Timing. **If** **analyzer 1** is already a timing analyzer, go on to step 3.
 - Place the cursor on the **Type:** _____ **field** and press SELECT.
 - Place the cursor on Timing and press **SELECT**.

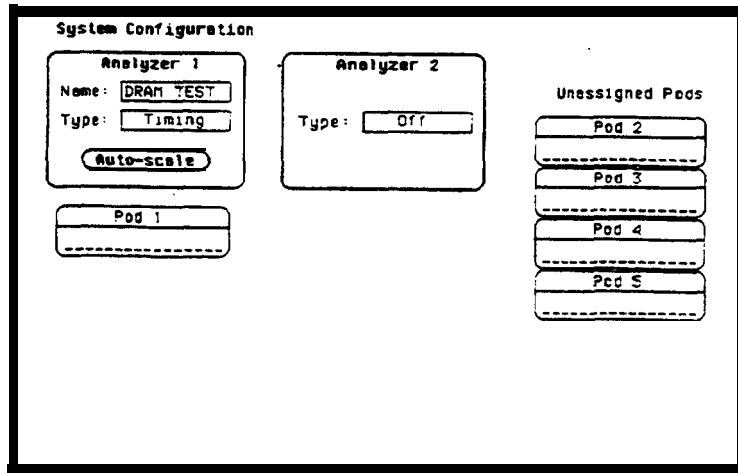

3.Name Analyzer 1 "DRAM TEST (optional)

- a. **Place** the cursor on the **Name: field** of **Analyzer 1** and press **SELECT**.
- b. **With** the **Alpha Entry** pop-up, change the name to **"DRAM TEST"** (see "Alpha Entry Pop-up Menu" in chapter 4 if you need a reminder).

4.Assign pod 1 to the timing analyzer.


- a. Place the cursor **on** the **Pod 1** held and press **SELECT**.
- b. In the **Pod 1** pop-up, place the cursor on **Analyzer 1** and press **SELECT**.

Connecting the Probes

At this point, if you had a target system with a 4116 DRAM memory IC, you would connect the logic analyzer to your system.

Since you will be assigning Pod 1 bit 0 to the RAS label, you connect Pod 1 bit 0 to the memory IC pin connected to the RAS signal. You connect Pod 1 bit 1 to the IC pin connected to the CAS signal.

Activity Indicators When the logic analyzer is connected and your target system is running, you will see **↑** at the right-most end (least significant bits) of the Pod 1 field in the System Configuration menu. This indicates the RAS and CAS signals are transitioning.

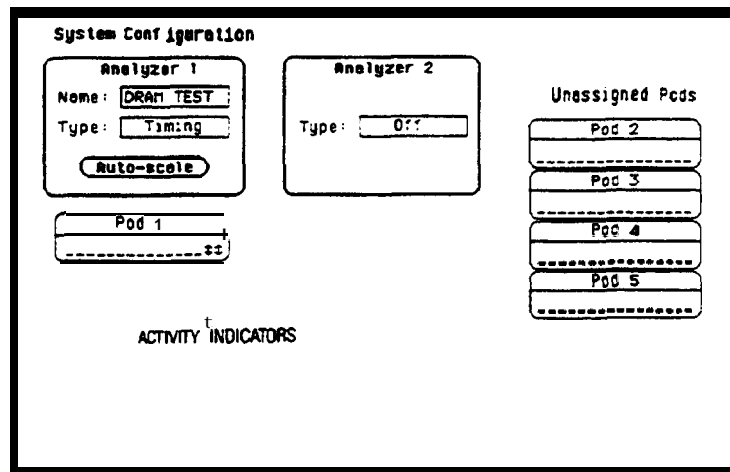

Configuring the Timing Analyzer

Now that you have **configured** the system, you are ready to **configure** the timing analyzer. You will be:

- **Creating** two names (labels) for the input signals
- **Assigning the channels connected to the input signals**
- **Specifying** a trigger condition


1. Display the TIMING FORMAT SPECIFICATION menu.

a. Press the FORMAT key on the front panel

2. Name two labels, one **RAS** and one CAS.

a. Place the cursor on the top **field** in the label column and press **SELECT**.

b. Place the cursor on Modify label and press **SELECT**.

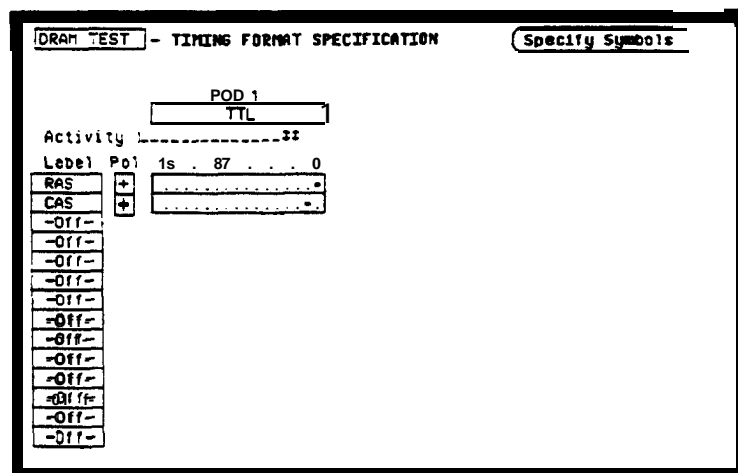

- c. With the Alpha Entry pop-up, change the name of the label to **RAS** (see “Alpha Entry Pop-up Menu” in chapter 4 if you need a reminder).
 - d. Name the second label **CAS** by repeating steps a through c.
 3. Assign the channels **connected** to the input signals (Pod 1 bit 0 and 1) **to the labels RAS and CAS** respectively.
 - a. Place the cursor on the bit assignment field below Pod 1 and to **the right of RAS and** press SELECT.
 - b. Any **combination** of bits may be **assigned** to this **pod**; however, you will want only bit 0 assigned **to the RAS label**. The easiest way to assign bits is to press the CLEAR ENTRY key to un-assign any **assigned** bits before you **start**.
 - c. Place the **cursor** on the period under the 0 in the bit assignment **pop-up** and press SELECT. This **will** place an **asterisk** in the pop-up for bit 0 indicating Pod 1 bit 0 is now assigned to the **RAS label**. Place cursor on Done and press **SELECT** to close **the pop-up**.
 - d. **Assign Pod 1 bit 1 to the CAS label by moving the cursor to bit 1 and pressing SELECT.**

Specifying a Trigger Condition

To capture the data **and** then place the data of interest in the center of **the** display of the TIMING WAVEFORMS menu, you need to **tell** the logic **analyzer** when to trigger. Since the first event of interest is when the **LRAS** is asserted (negative-going edge of RAS), you need to tell the logic **analyzer** to trigger on a negative-going edge of the RAS signal.


1. **Select** the TIMING TRACE menu by pressing the TRACE key.
2. Set the trigger so that the logic analyzer triggers on the negative-going edge of the **RAS**.
 - a. **Place** the cursor on the **Then find** Edge field under the **label** RAS, then press **SELECT**.
 - b. Place the cursor on the (period) in the pop-up **and** press **SELECT** once. **Pressing SELECT** once in this pop-up **changes** a period to **↓** which indicates a negative-going edge.
 - c. Place the cursor on Done and press **SELECT**. The **pop-up closes and a \$ will be located in this field. The \$ indicated an** edge has been **specified** even though it can't be shown in the **HEX base**.

The screenshot shows the 'DRAM TEST - TIMING TRACE SPECIFICATION' menu. The settings are as follows:

- Trace mode: Single
- Armed by: Run
- Acquisition mode: Transitions
- Label >: RAS | CAS
- Base >: Hex | Hex
- Find Pattern: X | X |
- present for >: 30 ns
- Then find Edge: \$

Acquiring the Data

Now that you have configured and connected the logic analyzer, you acquire the data for your measurement by pressing the RUN key. The logic analyzer will look for a negative edge on the RAS signal and trigger if it sees one. When it triggers, the display switches to the TIMING WAVEFORMS menu.

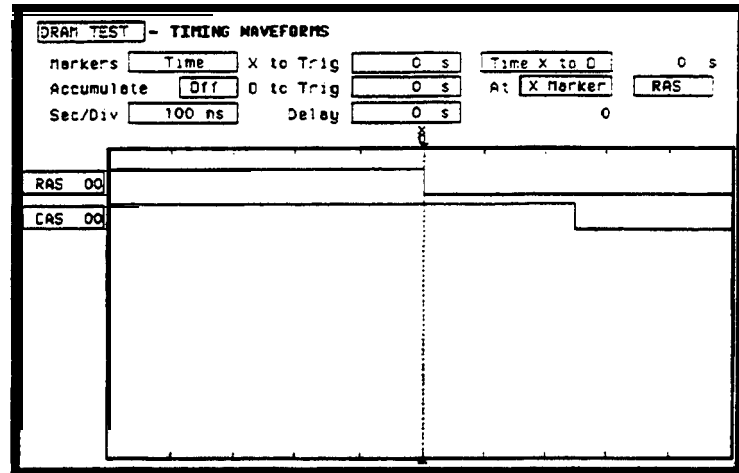

The RAS label shows you the RAS signal and the CAS label shows you the CAS signal. Notice the RAS signal goes low at or near the center of the waveform display area (horizontal center).


Now is the time to load the timing measurement demo file from the disk if you wish. The file name is TIMINGDEMO. Follow the procedure in Appendix B to load the file.

The Timing Waveforms Menu

The **TIMING WAVEFORMS** menu differs from the other menus you have **used** so far in this exercise. Besides displaying the acquired data, it has menu **fields** that you use **to** change the way the **acquired** data is displayed and fields that give you timing answers. Before you can use this menu to **find** answers, you need to know some of the special symbols and their functions. The symbols are:


- The **X** and **O**
- The **▼**
- The **vertical** dotted line

The X and O The X and O are markers you use to find your answer. You place them on the points of interest on your waveforms, and the logic **analyzer** displays the time between the markers. The X and O markers will be in the center of the display when X to **trig(ger)** and O to **trig(ger)** are both 0.000 s (see example below).

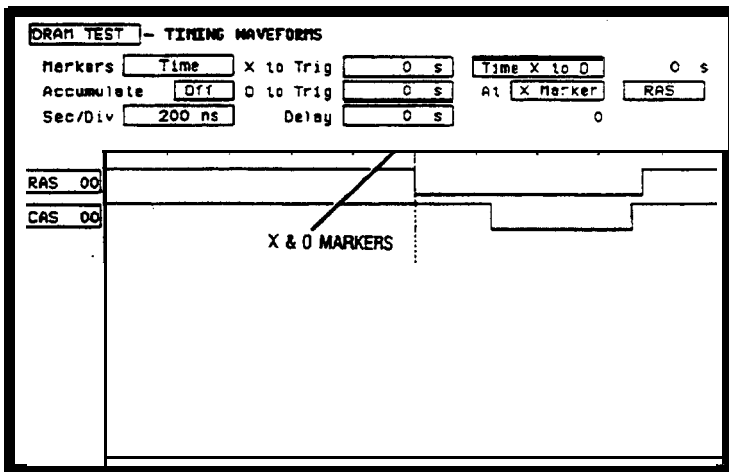

The ▼ The ▼ (inverted triangle) indicates the trace point. Remember, trace point = trigger + delay. Since delay in this example is 0.000 s, you will see the negative-going edge of the RAS signal at center screen under the ▼.

The Vertical Dotted line The vertical dotted line indicates the trigger point you specified in the TIMING TRACE SPECIFICATION menu. The vertical dotted line is at center screen under the ▼ and is superimposed on the negative-going edge of the RAS signal as shown.

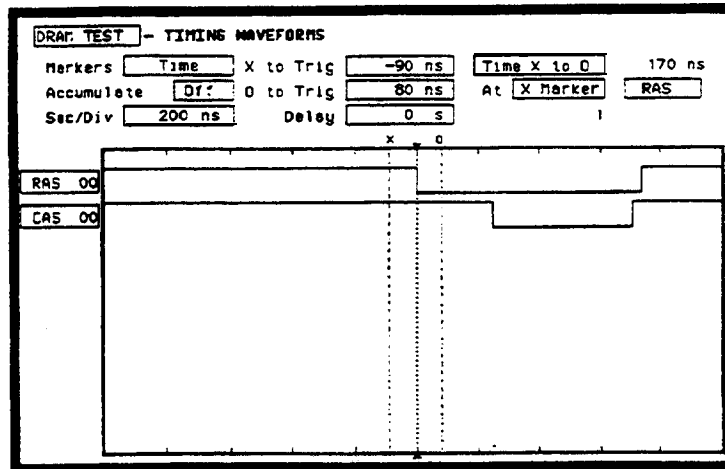

Configuring the Display


Now that you have acquired the RAS and CAS waveforms, you need to configure the TIMING WAVEFORMS menu for best resolution and to obtain your answer.

Display Resolution

You get the best resolution by changing the Sec/Div to a value that displays one negative-going edge of both the RAS and CAS waveforms. Set the Sec/Div by following these steps.




1. Place the cursor on **Sec/Div** and press **SELECT**. The **Sec/Div** pop-up appears, showing you the current setting.
- 2 While the pop-up is present, rotate the **KNOB** until your waveform shows you only one negative-going edge of the RAS waveform and one positive-going edge of the CAS waveform. (see above). In this example 200 ns is best.

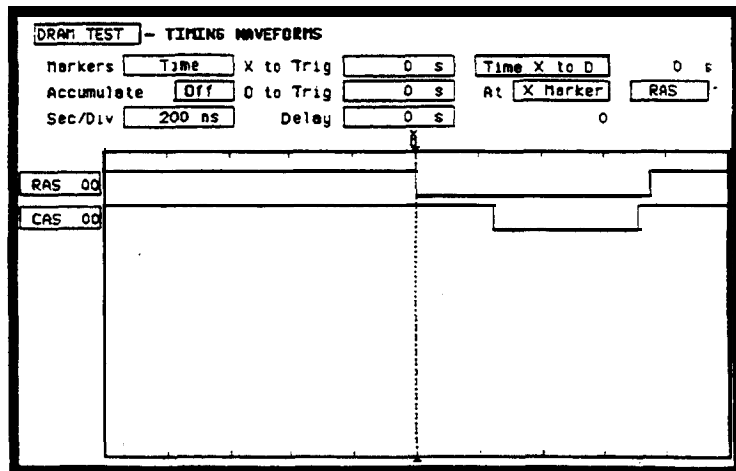

Making the Measurement

What you want to know is how much time elapses between the time RAS goes low and the time CAS goes high again. You will use the X and 0 markers to quickly find the answer. Remember, you specified the negative-going edge of the RAS to be your trigger point; therefore, the X marker should be on this edge if X to Trig = 0. If not, follow steps 1 and 2.


- 1 Place the cursor on the X to Trig field and press SELECT. A pop-up will appear showing you the current time from the X marker to the trigger; however, you don't need to worry about this number now.
- 2 Rotate the KNOB to place the X marker on the negative-going edge of the RAS waveform and press SELECT. The pop-up closes and displays X to Trig = 0.000 s.
- 3 Place the cursor on 0 to Trig and press SELECT. Repeat step 2 except place the 0 marker on the positive-going edge of the CAS waveform and press SELECT. The pop-up closes and displays O to Trig = 710 ns.

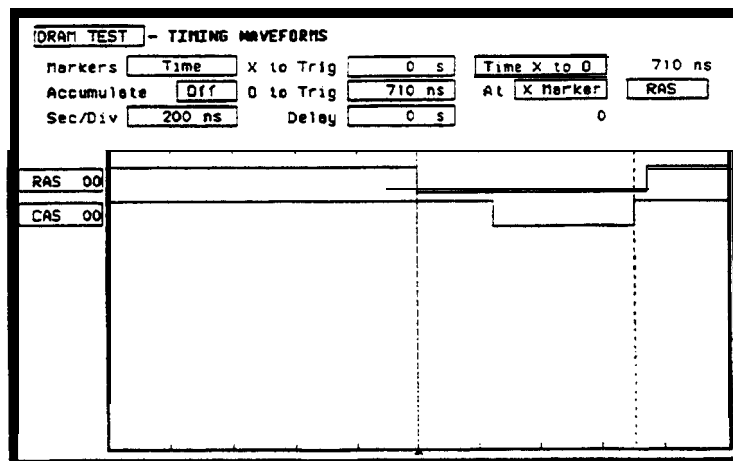

Finding the Answer

Your answer could be calculated by adding the X to Trig and O to Trig times, but you don't need to bother. The logic analyzer has already calculated this answer and displays it in the Time X to O _____ field.

This example indicated the time is 710 ns. Since the data book specifies a minimum of 250 ns, it appears your DRAM controller circuit is designed properly.

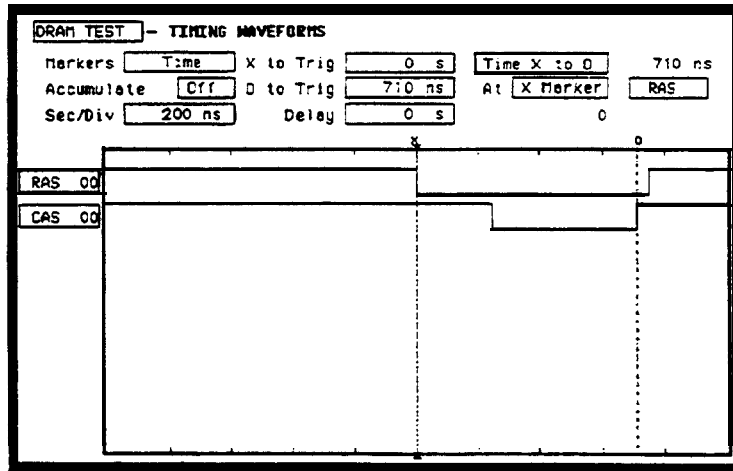

Summary

You have just learned how to make a simple timing measurement with the HP **1650B/51B** logic analyzer. You have:

- specified a timing analyzer
- **assignedpod1**
- **assignedbits**
- **assigned labels**
- **specified** a trigger condition
- learned which probes to **connect**
- **acquired the data**
- **configured** the display
- **set** the **Sec/Div** for best resolutions
- positioned the markers for the measurement answer

You have seen how easy it is to use the timing analyzer to make timing measurements that you could have made with a scope. You can use the timing analyzer for any timing measurement that doesn't require voltage **parametrics** or doesn't go beyond the accuracy of the timing analyzer.

The next chapter teaches you how to use the state analyzer. You will go through a simple state measurement **in** the same way you did the **timing** measurement in this **chapter**.

Using the State Analyzer

Introduction

In this chapter you will learn how to use the state analyzer by setting up the logic analyzer to make a simple state measurement. We give you the measurement results as actually measured by the logic analyzer, since you may not have the same circuit available.

The exercise in this chapter is organized in a task format. The tasks are in the same order you will most likely use them once you become experienced. The steps in this format are both numbered and lettered. The numbered steps state the step objective. The lettered steps explain how to accomplish each step objective. There is also an example of each menu after it has been properly set up.

How you use the steps depends on how much you remember from chapters 1 through 4. If you can set up each menu by just looking at the menu picture, go ahead and do so. If you need a reminder of what steps to perform, follow the numbered steps. If you still need more information about "how," use the lettered steps.

When you have finished configuring the logic analyzer for this exercise, you can load a file from the operating system disk. This file configures the logic analyzer the same way it is configured for this exercise. It also loads the same data acquired for this exercise so you can see what it looks like on screen.

In order to learn how to configure the logic analyzer, we recommend that you follow the exercise to "Acquiring the Data" before loading the file from the disk.

You can also compare your configuration with the one on the disk by printing it (if you have a printer) or making notes before you load the file.

Problem Solving with the State Analyzer

In this example assume you have designed a microprocessor **controlled circuit**. You have completed the hardware, and the software designer has completed the software and programmed the ROM (read-only memory). When you **turn** your circuit on for the **first time**, your circuit **doesn't work properly**. You have checked the power supply voltages and the system clock and they are **working properly**.

Since the circuit has never worked before, you and the software engineer aren't sure if it is a hardware or software problem, You need to do some testing to **find** a solution

What Am I Going to Measure?

You decide to start where the microprocessor starts when power is applied. We will describe a 68000 microprocessor, however, every processor has similar start-up routines.

When you power up a 68000 microprocessor, it is held in reset for a **specific length of time** before it starts **doing anything to stabilize the** power supplies. The **time the microprocessor** is held in reset ensures **stable levels (states) on all the devices and buses in your circuit**. When this reset period has ended, the 68000 performs a **specific routine** called "fetching **the reset vector**."

The **first** thing you check is the time the microprocessor is held in reset. You find the time is **correct**. The next thing to check is whether the microprocessor fetches the reset vector properly.

The steps of the 68000 reset vector fetch are:

1. Set the stack pointer to a location you specify, which is in ROM at address locations 0 and 2.
2. Find the first address location in memory where the microprocessor fetches its first **instruction**. This is also specified by you and stored in ROM at address locations 4 and 6.

What you decide to **find out is:**

1. **What ROM address does the microprocessor look at for the location of the stack pointer, and what is the stack pointer location stored in ROM?**
2. **What ROM address does the microprocessor look at for the address where its first instruction is stored in ROM, and is the instruction correct?**
3. **Does the microprocessor then go to the address where its first instruction is stored?**
4. **Is the executable instruction stored in the first instruction location correct?**

Your **measurement, then,** requires verification of the sequential addresses the **microprocessor** looks at, and of the data in ROM at these addresses. If **the reset vector fetch is correct (in this example),** you will see the following list of numbers in HEX (default base) when your measurement results are displayed

```
+0000 000000 0000
+0001 000002 04FC
+0002 000004 0000
+0003 000006 8048
+0004 008048 3E7C
```


This list of numbers will be explained in detail later in this chapter in "The State Listing."

How Do I Configure the Logic Analyzer?

In order to make this **state** measurement, you must **configure** the logic analyzer as a state analyzer. By following these steps you will **configure Analyzer 1 as the state analyzer**.

If you are in the **System Configuration** menu you are in the **right** place to get **started** and you can start with step **2**; otherwise, start with step **1**.

1. Using the field in the upper left corner of the display, get the **System Configuration** menu **on screen**.
 - a. **Place the cursor** on the field in the upper left corner of the display and press **SELECT**.
 - b. **Place the cursor** on **System** and press **SELECT**.
2. In the **System Configuration** menu, change the **Analyzer 1** type to **State**. If **Analyzer 1** is already a **state analyzer**, go on to step 3.
 - a. **Place the cursor** on the **Type: _____** and press **SELECT**.
 - b. **Place the cursor** on **State** and press **SELECT**.

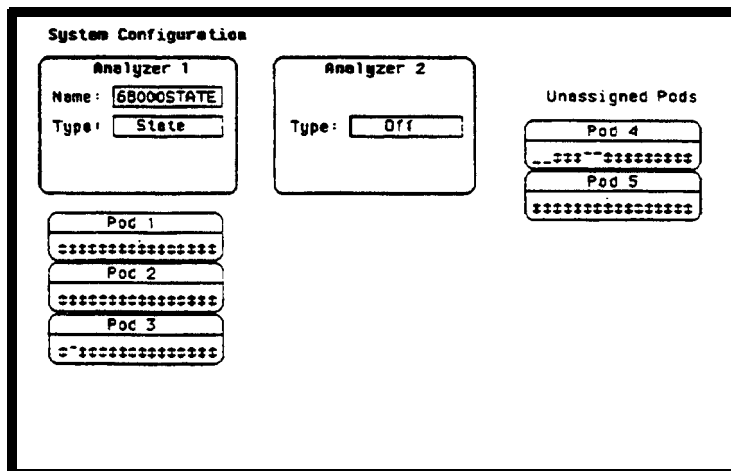

3. Name Analyzer 1 68000STATE (optional)

- a. Place the **cursor** on the **Name: _____** field of Analyzer 1 and press **SELECT**.
- b. With the Alpha Entry pop-up, change the name to **68000STATE** (see “Alpha Entry Pop-up Menu” in chapter 4 if you need a reminder).

4. Assign pods 1, 2, and 3 to the state analyzer.

- a. Place the **cursor** on the Pod 1 field and press **SELECT**.
- b. In the Pod 1 pop-up, place the cursor on **Analyzer 1** and press **SELECT**.
- c. Repeat steps a and b for pods 2 and 3.


Connecting the Probes

At this point, if you had a target system with a **68000** microprocessor, you would **connect** the logic **analyzer** to your **system**. **Since** you will be **assigning** labels ADDR and DATA, you conned the probes to your **system accordingly**.

- Pod 1 probes 0 through **15** to the **data** bus lines DO through **D15**.
- Pod 2 probes 0 through **15** to the address bus lines **A0** through **A15**.
- Pod 3 probes 0 through 7 to the address bus **lines** A16 through **A23**.
- Pod **1**, **CLK** (J clock) to the address strobe (LAS).

Activity Indicators

When the logic **analyzer** is **connected** and your target **system** is running, you will see **↑** in the Pod **1, 2,** and 3 fields of the System Configuration menu. This **indicates which signal** lines are **transitioning**.

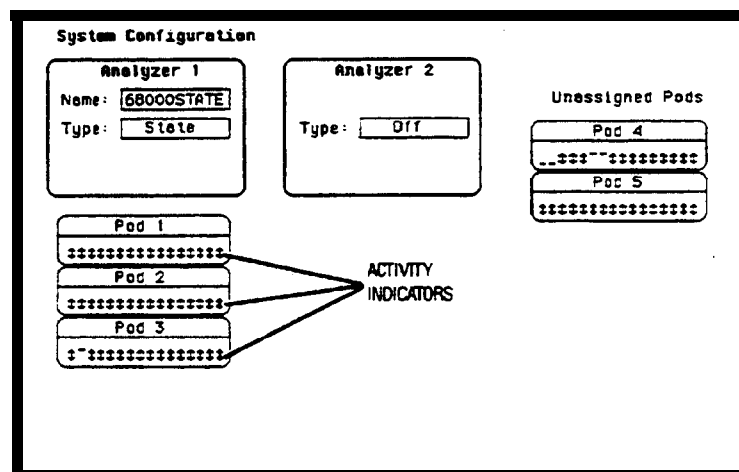


Configuring the State Analyzer

Now that you have configured the system, you are ready to configure the state analyzer. You will be:

- Creating two names (labels) for the input signals
- Assigning the channels connected to the input signals
- Specifying the State (J) clock
- Specifying a trigger condition

1. Display the STATE FORMAT SPECIFICATION menu.
 - a. Press the FORMAT key on the front panel.
2. Name two labels, one ADDR and one DATA.
 - a. Place the cursor on the top field in the label column and press SELECT.
 - b. Place the cursor on **Modify** label and press SELECT.

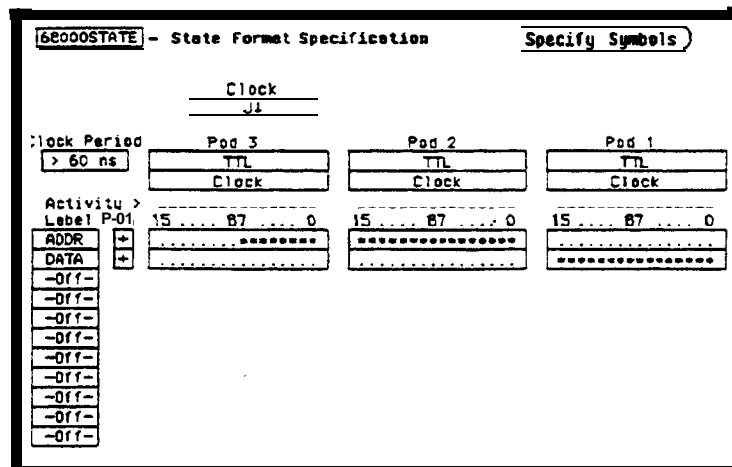

c. With the Alpha Entry pop-up, change the name of the label to ADDR (see "Alpha Entry Pop-up Menu" in chapter 4 if you need a reminder).

d. Name the second label DATA by repeating steps a through c

3. Assign Pod 1 bits 0 through 15 to the label DATA

a. Place the cursor on the bit assignment field below Pod 1 and to the right of DATA and press SELECT.

b. Any combination of bits may already be assigned to this pod; however, you will want all 16 bits assigned to the DATA label. The easiest way to assign is to press the CLEAR ENTRY key to un-assign any assigned bits before you start.

c. Place the cursor on the period under the 15 in the bit assignment pop-up and press SELECT. This will place an asterisk in the pop-up for bit 15, indicating Pod 1 bit 15 is now assigned to the DATA label. Repeat this procedure until all 16 bits have an asterisk under each bit number. Place the cursor on Done and press SELECT to close the pop-up.


d. Repeat step c for Pod 2 and the ADDR label to assign all 16 bits.

e. Repeat step c except you will assign the lower eight bits (0 - 7) of Pod 3 to the ADDR label.

Specifying the J Clock

If you remember from "What's a State Analyzer" in *Feeling Comfortable With Logic Analyzers*, the state analyzer samples the data under the control of an external clock, which is "synchronous" with your circuit under test. Therefore, you must specify which clock probe you will use for your measurement. In this exercise, you will use the J clock, which is accessible through pod L.

1. Select the STATE FORMAT SPECIFICATION menu by pressing the **FORMAT** key.
- 2 Set the J Clock to sample on a negative-going edge.
 - a. Place the cursor on the **CLOCK** field and press **SELECT**.
 - b. Place the cursor on the box just to the right of **J** in the pop-up (labeled **OFF**) and press **SELECT**.
 - c. Place the cursor on **↓** and press **SELECT**.
 - d. Place the cursor on **Done** and press **SELECT**.

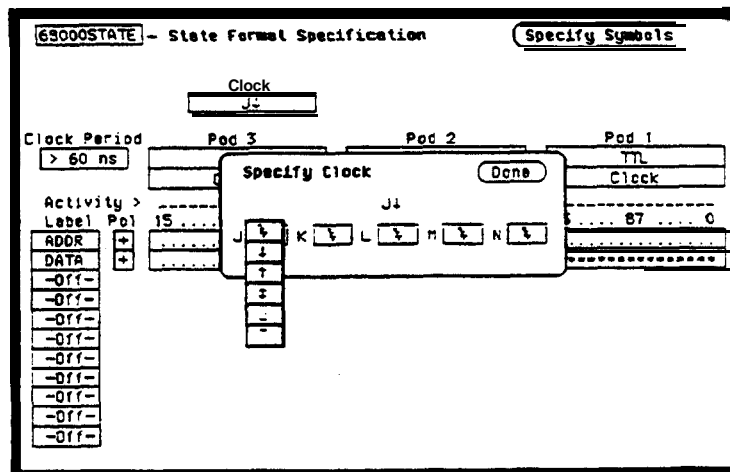

Specifying a Trigger Condition

To capture the data and place the data of interest in the center of the display of the STATE LISTING menu, you need to tell the state analyzer when to trigger. Since the first event of interest is address 0000, you need to tell the state analyzer to trigger when it detects address 0000 on the address bus.

1. Select the STATE TRACE SPECIFICATION menu by pressing the TRACE key.
2. Set the trigger so that the state analyzer triggers on address 0000.
 - a. Place the cursor on the 1 in the Sequence Levels field of the menu and press SELECT.

The screenshot shows the STATE TRACE SPECIFICATION menu with the following fields and options:

- Trace mode: Single
- Sequence Levels: 1 (selected), 2
- Armed by: Run
- Sequence Level 1: Done
- Insert Level: []
- Delete Level: []
- While storing anystate: []
- Trigger on: [] 1 times
- Label Base:

	Hex	Hex
a	000000	0000
b	XXXXXXXX	XXXXX
c	XXXXXXXX	XXXXX
c	XXXXXXXX	XXXXX
- Branches: Off
- Count: Off
- Restore: Off

- b. Place the cursor on the anystate field to the right of the Trigger on field and press SELECT. Another pop-up appears showing you a list of “trigger on” options. Options a through h are qualifiers. You can assign them a pattern for the trigger specification.

- c. Place the cursor on the **a** option and press **SELECT**.
- d. Place the cursor on **Done** in the **Sequence Levels** pop-up and press **SELECT**.
- e. Place the cursor on the field to the right of the **a** under the label **ADDR** and press **SELECT**.
- f. With the keypad, press **0 (zero)** until there are all zeros in the **Specify Pattern:** pop-up and then press **SELECT**.

Your **trigger specification** now states: **While storing anystate, trigger on "a" once and then store anystate.**"

The screenshot shows the STATE TRACE SPECIFICATION screen. At the top, it says '158000STATE :- STATE TRACE SPECIFICATION'. Below that, 'Trace mode' is set to 'Single'. The 'Sequence Levels' section shows a flowchart with two levels: Level 1 is 'While storing "anystate" Trigger on "a" : times' and Level 2 is 'Store "anystate"'. To the right, there are controls for 'Armed by' (Run), 'Branches' (Off), 'Count' (Off), and 'Prestore' (Off). At the bottom, there is a table with columns 'Label >', 'Base >', 'ADDR', and 'DATA'. The table contains four rows of data, with the first row showing '0' and '000000'.


Label >	Base >	ADDR	DATA
		Hex	Hex
a		000000	0000
b		XXXXXXXX	XXXX
c		XXXXXXXX	XXXX
d		XXXXXXXX	XXXX

When the state analyzer is connected to your circuit and is acquiring data, it continuously stores until it sees **0000** on the address bus, then it will store **anystate** until the analyzer memory is filled.

Acquiring the Data

Since you want to capture the data when the **microprocessor** sends address 0000 on the bus after power-up, you press the **RUN** key to arm **the** state analyzer and then force a reset of your circuit. When the reset cycle ends, the microprocessor should send address 0000, **trigger** the state analyzer and switch the display to the STATE **LISTING** menu

We'll assume this **is what** happens **in** this example, since the odds that the microprocessor won't send address 0000 are **very** low.

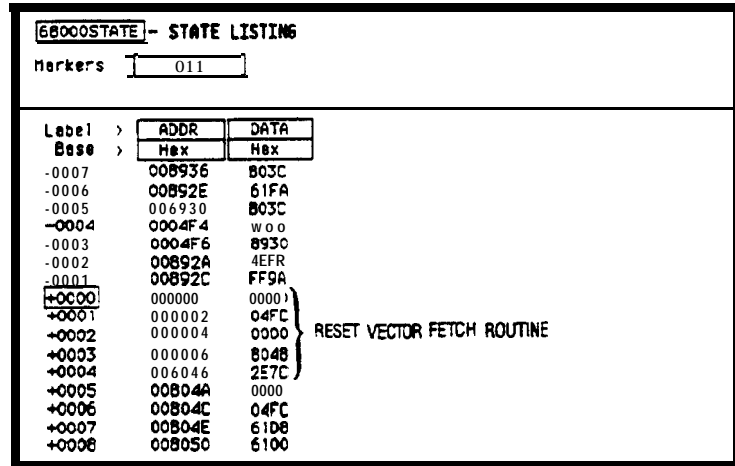


```
68000STATE]- STATE LISTING
Markers 011

Label > ADDR DATA
Base > Hex Hex
-0007 008936 803C
-0006 00892E 61FA
-0005 006930 803C
-0004 0004F4 W00
-0003 0004F6 8930
-0002 00892A 4EFA
-0001 00892C FF9A
+0000 000000 0000
+0001 000002 04FC
+0002 000004 0000 } RESET VECTOR FETCH ROUTINE
+0003 000006 804B
+0004 006046 2E7C
+0005 00804A 0000
+0006 00804C 04FC
+0007 00804E 61D8
+0008 008050 6100
```

Now is the time to load the state measurement demo file from the disk if you wish. The **file** name **is** STATEDEMO. Follow the procedure in Appendix B to load the **file**.

The State Listing

The state listing displays three columns of numbers as shown:

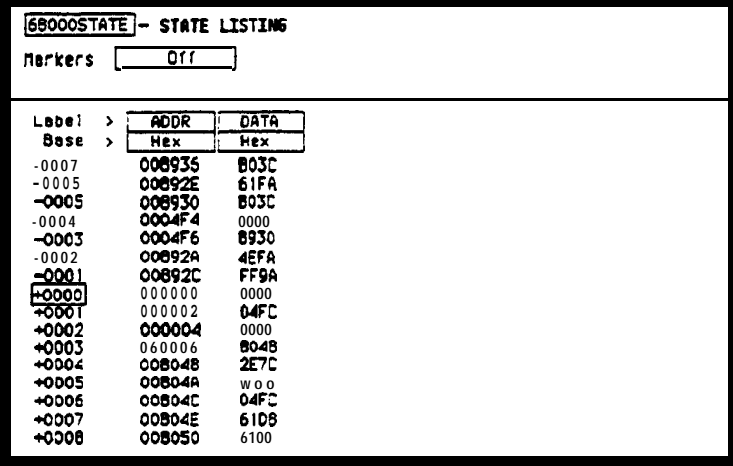

The screenshot shows a window titled "65000STATE - STATE LISTING". Below the title bar, there is a "Markers" field with the value "Off". The main content is a table with three columns: "Label", "ADDR", and "DATA". The "Label" column contains state line numbers ranging from -0007 to +0008. The "ADDR" and "DATA" columns contain hexadecimal values. The row for state +0000 is highlighted.

Label	ADDR	DATA
Base	Hex	Hex
-0007	008935	803C
-0005	00892E	61FA
-0005	008930	803C
-0004	0004F4	0000
-0003	0004F6	8930
-0002	00892A	4EFA
-0001	00892C	FF9A
+0000	000000	0000
+0001	000002	04FC
+0002	000004	0000
+0003	060006	8048
+0004	008048	2E7C
+0005	00804A	W00
+0006	00804C	04FC
+0007	00804E	6108
+0008	008050	6100

STATE LOCATIONS

The first column of numbers are the state line number locations as they relate to the trigger point. The trigger state is on line + 0000 in the vertical center of the list area. The negative numbers indicate states occurring before the trigger and the positive numbers indicate states occurring after the trigger.

The second column of numbers are the states (listed in HEX) the state analyzer sees on the address bus. This column is labeled ADDR

The third column of numbers are the states (listed in HEX) the state analyzer sees on the data bus. This column is labeled DATA.

Finding the Answer

Your answer is now found in the listing of states +0000 through +0004.

The 68000 **always** reads address locations 0, 2, 4, and 6 to find the stack pointer location and memory location for the **instruction** it fetches after power-up. The 68000 uses two words for each of the locations that it is looking for, a high word and a low word- **When** the software designer programs the ROM, **he** must put the stack pointer location at address **locations 0 and 2. 0 is the high word location and 2 is the low word location.** Similarly, the high word of the instruction **fetch** location **must be in address location 4 and the low word in location 6.**

Since the software design calls for the reset vector to:

1. set the stack pointer to **04FC**
2. read memory address location 8048 for its first instruction fetch,

you are interested in what is on both the address bus and the data bus in states 0 through 3. You look at the following listing and see that states 0 and 1 do contain address locations 0 and 2 under the ADDR label, indicating the **microprocessor** did look at the correct locations for the stack pointer data. You also see that the data contained in these ROM locations are 0000 and **04FC**, which are **correct.**

You then **look** at states 2 and 3. You **see** that the next two address locations are 4 and 6, which is correct, and the data found at these **locations is 0000 and 8048, which is also correct.**

```
+0000 000000 0000
+0001 000002 04FC
+0002 000004 0000
+0003 000006 8048
+0004 008048 3E7C
```

So far you have verified that the microprocessor has **correctly** performed the reset vector **search**. The next thing **you** must **verify** is **whether the microprocessor addresses the correct location in ROM that it was instructed to address in state 4 and whether the data is correct in this ROM location**. From the listing you see that the **address in state 4 is 008048, which is correct, but the instruction found in this location is 2E7C, which is not correct**. You have found your problem: **incorrect** data stored in ROM for the microprocessor's first instruction.

- +00a0 000000 0000 (high word of stack pointer location)
- +0001 W002 04FC (low word of stack pointer location)
- +0002 000004 0000 (high word of instruction fetch location)
- +0003 000006 8048 (low word of instruction fetch location)
- +0004 008048 2E7C (first microprocessor instruction)

68000STATE - STATE LISTING		
Markers	Off	
Label >	ADDR	DATA
Base >	Hex	Hex
-0007	008936	B0W
-0006	00892E	61FA
-0005	0 0 6 9 3 0	803C
-0004	0004F4	W 0 0
-0003	0004F6	8930
-0002	00892A	4EFA
-0001	00892C	FF9A
+0000	000000	0000
+0001	000002	04FC
+0002	000004	0000
+0003	000006	8048
+0004	008048	2E7C ← INCORRECT DATA
+0005	00804A	0000
+0006	00804C	04FC
+0007	00804E	61D8
+0008	008050	6100

Summary

You have just learned how to make a simple state measurement with the HP 1650B Logic Analyzer. You have:

- specified a state analyzer
- learned which probes to connect
- assigned pods 1, 2, and 3
- assigned labels
- assigned bits
- specified the J clock
- specified a trigger condition
- acquired the data
- interpreted the state listing

You have seen how easy it is to use the state analyzer to capture the data on the address and data buses. You can use this same technique to capture and display related data on the microprocessor status, control, and various strobe lines. You are not limited to using this technique on microprocessors. You can use this technique any time you need to capture data on multiple lines and need to sample the data relative to a system clock.

The next chapter teaches you how to use the logic analyzer as an interactive timing and state analyzer. You will see a simple measurement that shows you both timing waveforms and state listings and how they are correlated.

If you have an HP 1651B, you do not have enough channels to simultaneously capture all the data for a 68000. But, since you probably aren't working with 16-bit microprocessors, this example is still valuable because it shows you how to make the same kind of measurement on an eight-bit microprocessor.

Using the Timing/State Analyzer

Introduction

In this chapter you will learn how to use the timing and state analyzers interactively by setting up the logic analyzer to make a simple measurement. We give you the measurement results as actually measured by the logic analyzer, since you may not have the same circuit available.

The exercise in this chapter is organized differently than the exercises in the two previous chapters. Since you have already set up both the timing and state analyzers, you should be ready to set them up for this measurement by looking at the menu pictures.

Any new set-ups in this exercise will be explained in task format steps like the previous chapters.

How you use the steps depends on how much you remember from chapters 1 through 4. If you can set up each menu by just looking at the menu picture, go ahead and do so. If you need a reminder of what steps to perform, follow the numbered steps. If you still need more information about "how," use the lettered steps.

When you have finished configuring the logic analyzer for this exercise, you can load a file from the operating system disk. This file configures the logic analyzer the same way it is configured for this exercise. It also loads the same data acquired for this exercise so you can see what it looks like on screen.

In order to learn how to configure the logic analyzer, we recommend that you follow the exercise to "Acquiring the Data" before loading the file from the disk.

You can also compare your configuration with the one on the disk by printing it (if you have a printer) or making notes before you load the file.

Problem Solving with the Timing/State Analyzer

In this example assume you have designed a microprocessor-controlled circuit. You have completed the hardware, and the software designer has completed the software and programmed the ROM (read-only memory). When you turn your circuit on for the first time, your circuit doesn't work properly. You have checked the power supply voltages and the system clock, and they are working properly.

Since the circuit has never worked before, you and the software engineer aren't sure if it is a hardware or software problem. You need to do some testing to find a solution.

You also notice the circuit fails intermittently. More specifically, it only fails when the microprocessor attempts to address a routine that starts at address 8930,

What Am I Going to Measure?

To see what might be causing the failure, you decide to start where the microprocessor goes to the routine that starts at address 8930.

The first thing you check is whether the microprocessor actually addresses address 8930. The next thing you check is whether the code is correct in all the steps in this routine.

Your measurement, then, requires verification of:

- whether the microprocessor addresses location 8930
- whether all the addresses within the routine are correct
- whether all the data at the addresses in the routine are correct


If the routine is correct, the state listing will display

```
+0000 008930 B03C
+0001 008932 61FA
+0002 008934 67F8
+0003 008936 B03C
+0004 00892E 61FA
```

How Do I Configure the Logic Analyzer?

In order to make this measurement, you must configure the logic analyzer as a state analyzer because you want to trigger on a specific state (8930). You also want to verify that the addresses and data are correct in the states of this routine.


Configure the logic analyzer so that Analyzer 1 is a state analyzer as shown:

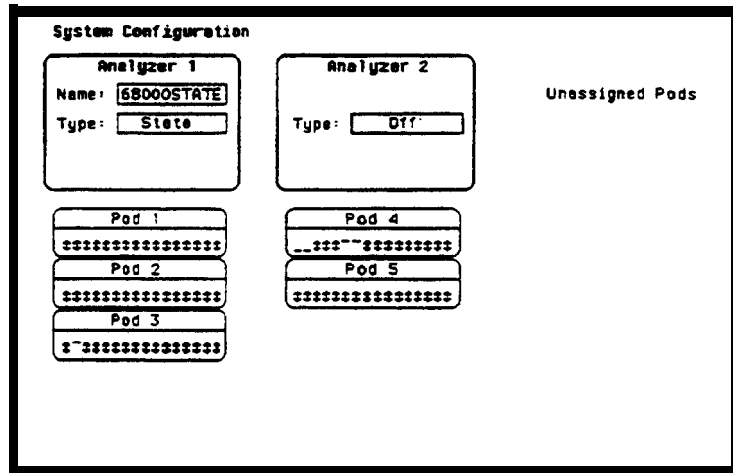


Configuring the State Analyzer

Now that you have configured the system, you are ready to configure the state analyzer.

Configure the STATE **FORMAT** SPECIFICATION menu as shown:

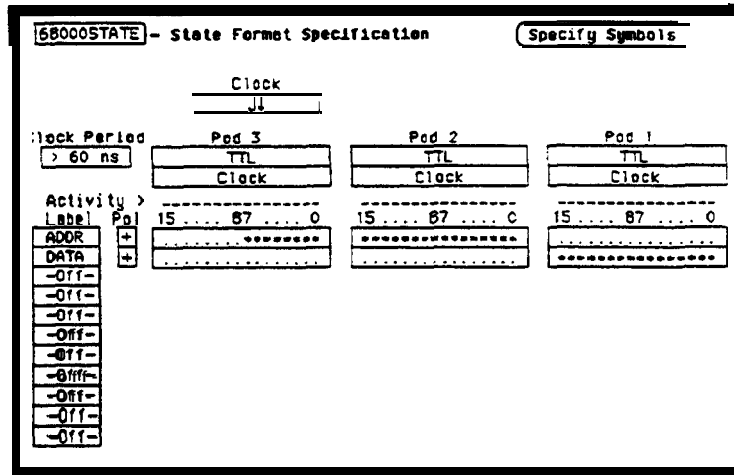

Configure the STATE TRACE SPECIFICATION menu as shown:

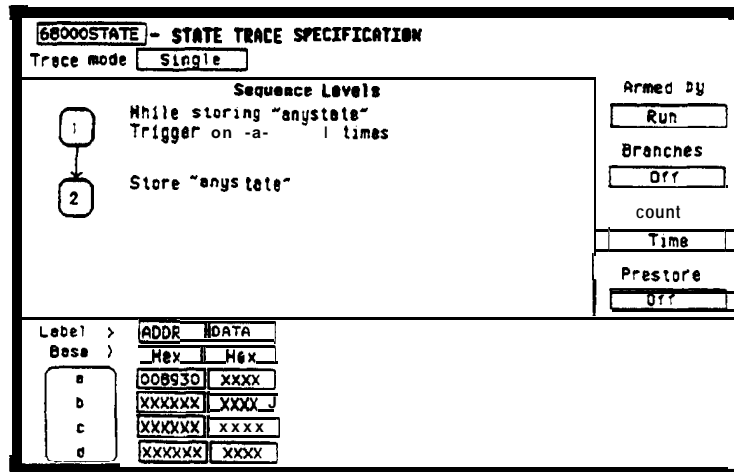

Connecting the Probes

At **this** point, if you had a target system with a 68000 microprocessor, **you would connect** the logic analyzer to your system. **Since you will be assigning labels** ADDR and DATA, you will hook the probes to your system accordingly.

- Pod 1 probes 0 through 15 to the data bus lines D0 through D15
- Pod 2 probes 0 through 15 to the address bus lines A0 through A15
- Pod 3 probes 0 through 7 to the address bus lines A16 through A23
- Pod 1, CLK (J clock) to the address strobe (LAS)

Acquiring the Data

Since you want to capture the data when the **microprocessor** sends address 8930 on the bus, you press the RUN key to arm the state analyzer. If the microprocessor sends address 8930, it will trigger the state analyzer and switch the display to the STATE LISTING menu.

We'll assume this is what happens in this example.

Finding the Problem

You look at this listing to see what the data is in states +0000 through +0004. You know your routine is five states long.

The 68000 does address location 8930, so you know that the routine is addressed. Now you **need** to compare the state listing with the following **correct** addresses and data:

```
+0000 008930 B03C
+0001 008932 61FA
+0002 008934 67F8
+0003 008936 B03C
+0004 00892E 61FA
```

As you compare the state **listing** (shown below) with the **above** data, you **notice** the data at address 8932 is **incorrect**. Now you need to find out **why**.

68000STATE - STATE LISTING		
narkrrs	Dff	
Label	ADDR	DATA
Base	Hex	Hex
4 0 0 7	0088CA	00FF
-0006	0088CC	6730
-0005	0088CE	48E7
-0004	0088FE	4E75
-0003	008900	3000
-0002	000284	0000
-0001	000286	0930
-0000	008930	B03C
4 0 0 1	006952	00FF
+0002	008954	67F8
+0003	008936	B03C
+0004	00892E	61FA
+0005	008930	B03C
+0006	000284	0000
+0007	000286	8930
+0008	00892A	4EFA

← INCORRECT DATA

Your **first** assumption is that incorrect data is stored to **this** memory location. Assume this routine **is** in ROM since it **is** part of the operating system for your **circuit**. Since the ROM is programmed by the software designer, you have the software designer **verify** whether or not the data at address 8932 is **correct**. The **software** designer tells you that the data is **correct**. Now what do you do?

Now it's time to **look** at the hardware to see if it is causing incorrect data when the microprocessor reads **this** memory address. You decide you want to see what is happening on the **address** and data **buses** during this routine in the time **domain**

In order to see the time domain, you need the timing analyzer.

What Additional Measurements Must I Make?

Since the problem exists during the routine that starts at address **8930**, you decide you **want** to see the timing waveforms **on** the address and data bus **when the routine is running**. You also want to see the control signals that control the **read** cycle. You will **then** compare the waveforms with the timing diagrams in the **68000 data book**.

Your measurement, then, requires **verification** of:

- **correct timing of the control signals**
- stable addresses and data during the memory read


The control signals you must check **are**:

- systemclock
- address strobe (AS)
- **lower** and upper data strobes (**LDS** and **UDS**)
- data transfer acknowledge (**DTACK**)
- read/write (**R/W**)

How Do I Re-configure the Logic Analyzer?

In order to make this **measurement**, you must **re-configure** the logic analyzer so **Analyzer 2 is a timing analyzer**. You leave **Analyzer 1 as a state analyzer** since you will use the state analyzer to trigger on address 8930.

Configure the logic analyzer so **Analyzer 2 is a timing analyzer** as shown:

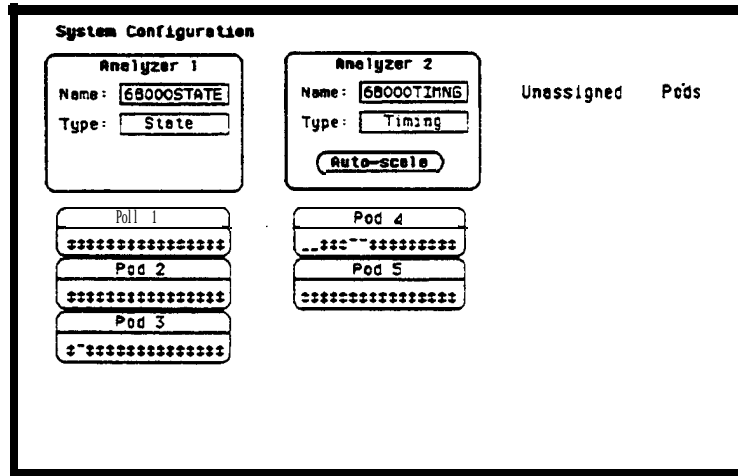

Connecting the Timing Analyzer Probes


At this point you would connect the probes of pods 4 and 5 as follows:

- Pod 4 bit 0 to address strobe (AS)
- **Pod 4 bit 1 to the system clock**
- Pod 4 bit 2 to low data strobe (LDS)
- Pod 4 bit 3 to upper data strobe (UDS)
- Pod 4 bit 4 to the **read/write** (R/W)
- Pod 4 bit 5 to data transfer acknowledge (DTACK)
- Pod 5 bits 0 through 7 to address lines **A0** through **A7**
- **Pod 5 bits 8 through 15 to data lines D0 through D7**


Configuring the Timing Analyzer

Now that you have configured the system, you are ready to configure the timing analyzer.

Configure the TIMING FORMAT SPECIFICATION menu as shown:

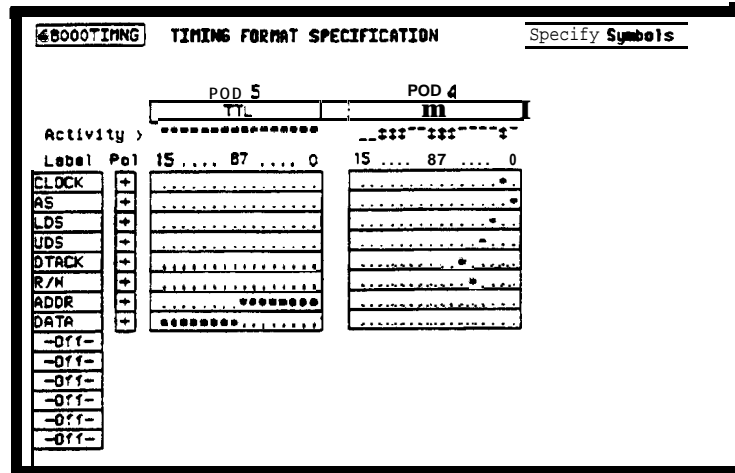

Configure the TIMING TRACE SPECIFICATION menu as shown:

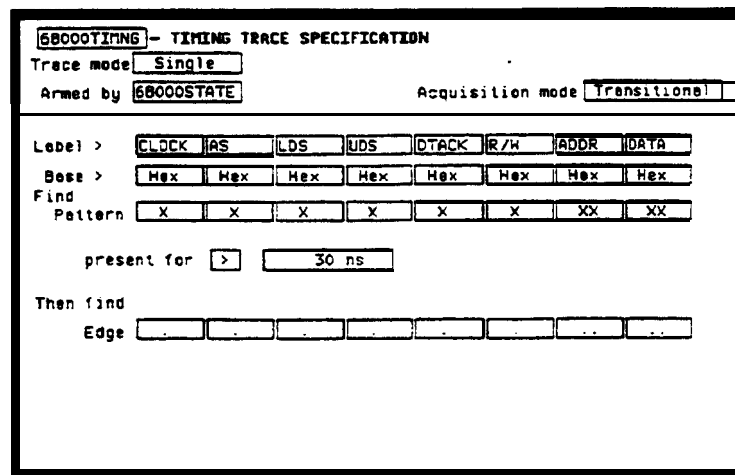

Setting the Timing Analyzer Trigger

Your timing measurement requires the timing analyzer to display the timing waveforms present on the buses when the routine is running. Since you triggered the state analyzer on address 8930, you want to trigger the timing analyzer so the timing waveforms can be time correlated with the state listing.

To set up the logic analyzer so that the state analyzer triggers the timing analyzer, perform these steps

1. Display the TIMING TRACE SPECIFICATION menu
2. Place the cursor on the Armed by field and press SELECT.
3. Place the cursor on the 68000STATE option in the pop-up and press SELECT.

Your timing trace specification should match the menu shown:

STATE ANALYZER
ARMS TIMING
ANALYZER

68000TIMING - TIMING TRACE SPECIFICATION

Trace mode Acquisition mode

Armed by

Label >

Base >

Find

Pattern

present for >

Then find

Edge

Time Correlating the Data

In order to time correlate the data, the logic analyzer must store the timing relationships between states. Since the timing analyzer samples asynchronously and the state analyzer samples synchronously, the logic analyzer must use the stored timing relationship of the data to reconstruct a time correlated display.

To set up the logic analyzer to keep track of these timing relationships, turn on a counter in the STATE TRACE SPECIFICATION menu. The following steps show you how,

1. Display the **STATE TRACE SPECIFICATION** menu
2. Place the cursor in the field just below **Count** on the right side of the display and press **SELECT**.
3. Place the cursor on the **Time** option and press **SELECT**. The counter will now be able to keep track of time for the time correlation.

The screenshot shows the '68000STATE' menu with the title 'STATE TRACE SPECIFICATION'. The 'Trace mode' is set to 'Single'. The 'Sequence Levels' section contains two steps: Step 1 is 'While storing "anystate" Trigger on "a" 1 times', and Step 2 is 'Store "anystate"'. On the right side, there are several control fields: 'Armed by' is set to 'Run', 'Branches' is 'Off', 'Count' is set to 'Time', and 'Prestore' is 'Off'. At the bottom, there is a table for labels and bases.

Label >	ADDR	DATA
Base >	Hex	Hex
a	008930	XXXX
b	XXXXXXXX	XXXX
c	XXXXXXXX	XXXX
d	XXXXXXXX	XXXX

Re-acquiring the Data

After you connect the probes of pods 4 and 5 to your circuit, all you have to do is press RUN. When the logic analyzer acquires the data, it switches the display to the STATE LISTING menu unless you switched one of the other menus to the timing analyzer after reconfiguring the STATE TRACE menu. Regardless of which menu is displayed, change the display to the Mixed mode.


Now is the time to load the mixed measurement demo file from the disk if you wish. The file name is MIXEDDEMO. Follow the procedure in Appendix B to load the file.

Mixed Mode Display

The Mixed mode display shows you both the STATE LISTING and TIMING WAVEFORMS menus simultaneously. To change the display to the Mixed mode:

1. Place the cursor on the field in the upper left corner of the display and press SELECT.
2. Place the cursor on Mixed mode and press SELECT.

You will now see the mixed display as shown:

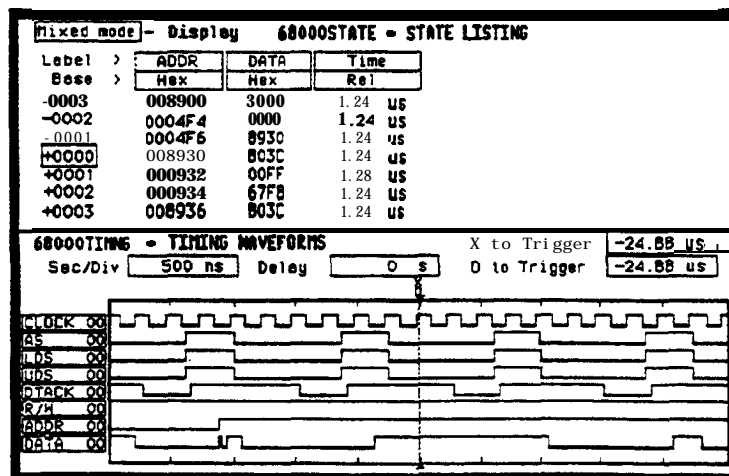


Interpreting the Display

In the **Mixed mode display** the state listing is in the top half of the screen and the **timing waveforms** are in the lower half. The important thing to remember is that you **time correlated** this display so you could see what is happening in the time domain during the faulty routine.

Notice that the trigger point in both parts of the display is the same as it was when the displays were separate. The trigger in the state listing is in the box containing **+0000** and the trigger of the timing waveform is the vertical dotted line.


As you look at the mixed display, you notice nothing wrong except the data at address **8932** is **incorrect**. However, you are seeing only one bit each of the address and the data. To see all the data and addresses in the timing waveform part of the display, you must overlap them.

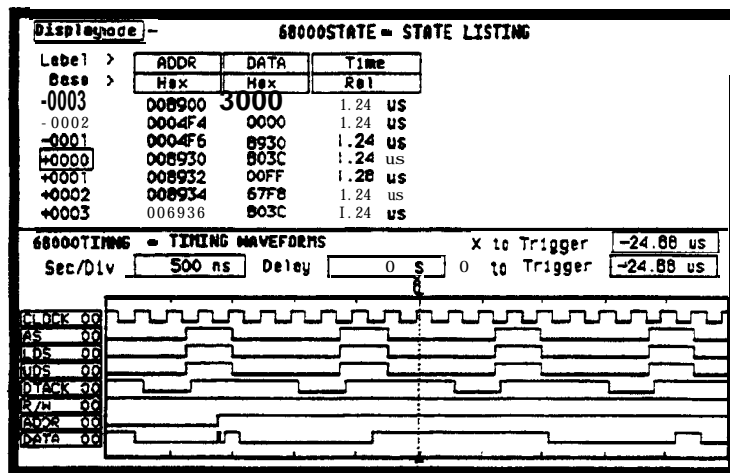

Overlapping Timing Waveforms


Since you see nothing wrong with the timing waveform so far, you think unstable data may be on the data lines during the read cycle. In order to see unstable data, you must be able to see all the data lines during the read and look for transitions. Overlapping the waveforms allows you to do this. To overlap waveforms, follow these steps:

1. Place the cursor on the 00 of the ADDR 00 label and press **SELECT**. The following pop-up opens in which you specify the bit or bits of the address bus you want to overlap.
2. Rotate the **KNOB** until **all** is displayed and press **SELECT**. All the address bits will be overlapped on one line.
3. Repeat step 2 except overlap the data bits.

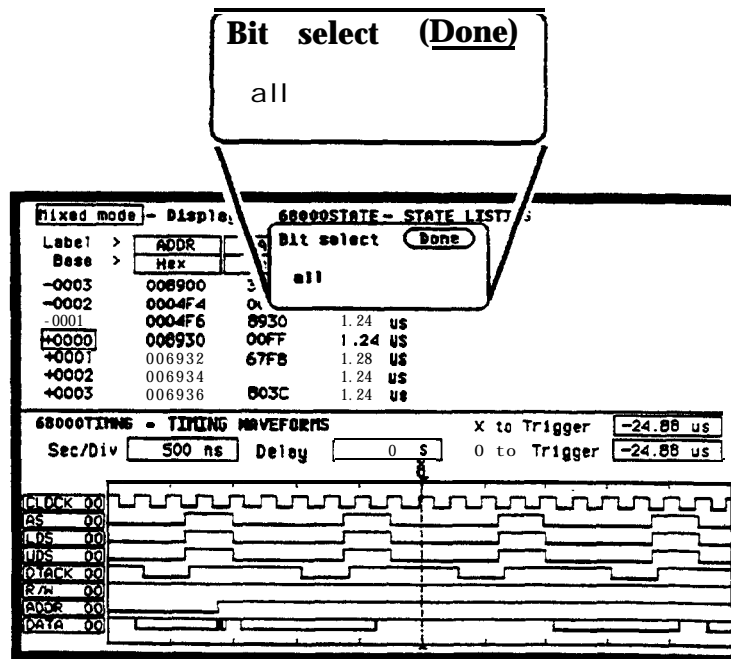

Finding the Answer

As you look at the overlapping waveforms, you notice there are transitions on the data lines during the read cycle, indicating the data is unstable. You have found the probable cause of the problem in this routine. Additional troubleshooting of the hardware will identify the actual cause.

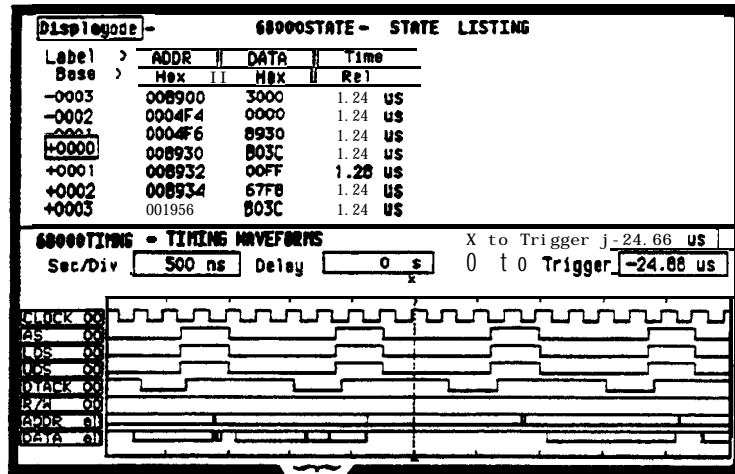

Summary

You have just learned how to use the timing and state **analyzers** interactively to **find** a problem that first appeared to be a software problem, but **actually** was a hardware problem.

You have **learned** to:

- trigger **one analyzer** with the other
- time correlate *measurement data*
- **interpret the Mixed mode display**
- overlap timing waveforms

If you have an **HP 1651B**, you do not have enough **channels** to simultaneously capture **all** the data for a **68000**. **But**, since you probably aren't working with **16-bit** microprocessors, **this** exercise is still valuable **because** it shows you how to make the same kind of measurement on an eight-bit microprocessor.

Making Hardcopy Prints

Introduction

The HP 1650B/51B Logic Analyzers allow you to print the configurations, waveforms, and listings. Whenever your printer is connected to your logic analyzer and you instruct it to do so, it will print what is currently displayed on screen.

This chapter shows you how to set up the logic analyzer's HP-IB and RS-232C interfaces for printers. If you have a Hewlett-Packard ThinkJet, QuietJet, or LaserJet series printer with the RS-232C interface, the RS-232C interface is already set up for you.

If you have another kind of printer, refer to your printer manual for its interface requirements and change your logic analyzer's interface configuration as instructed.

Hooking Up Your Printer

If your printer is already connected to the logic analyzer, skip to "Setting RS-232C for HP Printers" or "Setting HP-IB for HP Printers." If not, hooking up your printer is just a matter of having the correct HP-IB or RS-232C interface cable. Refer to the *Front-Panel Reference manual* you received with your logic analyzer.

Setting RS-232C for HP Printers

As you have to do to set the interface for any of the previously listed Hewlett-Packard series printers with the RS-232C interface is to set the printer type in the External I/O Port Configuration submenu.

To set the printer type, follow these steps:

1. Display the I/O menu by pressing the I/O key.
2. Place the cursor on I/O Port Configuration and press SELECT.


You will see the following submenu:

The screenshot shows the 'External I/O Port Configuration' menu. At the top right is a 'Done' button. Below it, 'Printer connected to' is set to 'RS-232-C' and 'Controller connected to' is set to 'HP-IB'. The menu is divided into three sections: 'RS-232-C Configuration' with fields for Protocol (XON/XOFF), Data Bits (8), Stop Bits (1), Parity (None), and Baud rate (9600); 'HP-IB Configuration' with an HP-IB Address field set to 7; and 'Printer Information' with Printer set to LaserJet and Paper width set to 8.5".

3. If the Printer connected to field displays RS-232C skip to step 4. Otherwise, place the cursor in the Printer connected to HP-IB field and press SELECT. The Printer connected to switches from HP-IB to RS-232C.
4. Place the cursor on the printer series type and press SELECT.
5. Place the cursor on Done and press SELECT. The logic analyzer will display the menu that was displayed when you selected the I/O menu.

Setting RS-232C for Your Non-HP Printer

The following attributes of the RS-232C interface **must** be set to the correct **configuration** for **your printer**:

- FV0t0W1
- number of data bits
- number of stop bits
- 
- Baud rate
- paper width

You can set all of these **attributes** for your printer by **following** this procedure:

1. Press the **I/O** key to display the **I/O** menu
2. Place the cursor on **I/O Port Configuration** and press **SELECT**.
3. Place **the cursor** on the attribute and press **SELECT**.
4. When **the pop-up is open**, place the cursor on the option your printer requires and press **SELECT**. The **pop-up closes**, placing your selection **in** the box Repeat this step for all attributes that you need to change.
5. Place the cursor on Done and press **SELECT**. The logic **analyzer will display the menu that was** displayed when you selected the **I/O menu**.

Setting **HP-IB** for HP Printers

The HP 1650B/51B interfaces directly with HP PCL printers supporting the printer command language. These printers must also support **HP-IB** and "Listen Always." Printers currently available from Hewlett-Packard with these features include:

- HP 2225A ThinkJet
- HP 2227B QuietJet
- HP 3630A option 002 PaintJet

Note



The printer must be in "Listen Always" when HP-IB is the printer interface.

The HP 1650B/51B HP-IB port does not respond to service requests (SRQ) when controlling a printer. The SRQ enable setting for the **HP-IB** printer has no effect on the **HP 1650B/1651B** operation.


For HP-IB printers, the Printer connect to field must be set to **HP-IB** in the **I/O Port Configuration** menu. You access the **I/O Port Configuration** menu by first accessing the **I/O menu**, then the **I/O Port Configuration**.

Starting the Printout

When you are ready to print, you will **need** to know whether there is more data than is displayed on screen. In cases where data is off screen (i.e., format specifications with all pods assigned to a single analyzer), you need to decide whether you want all the data or just the data is on screen.

If you want just what is on screen, start the printout with the **Print Screen** option. If you want all the data, use the **Print All** option. Both options are in the **I/O** menu.

Once you decide which option to use, **start** the printout by placing the cursor on the print option (screen or all) and pressing **SELECT**.

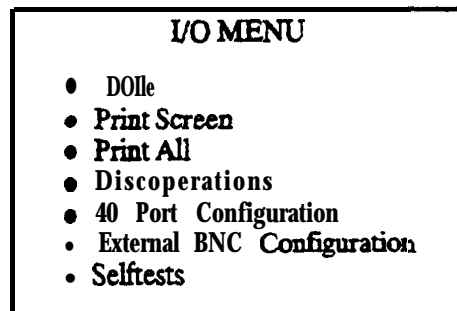

Print Screen The **Print Screen** option prints only what is displayed on screen at the time you initiate the printout. In the **Print Screen** mode, the printer **uses** its graphics capabilities so the printout will look just like the logic analyzer screen with only one exception: the cursor will not **print**.

Print All The **Print all option prints** not **only what is displayed on screen**, but also **what** is off screen at the time you initiate the printout. **In** the Print **All mode, the printout will be made in the text mode with only one exception:** a timing waveform display will be printed in the **graphics mode** because it has no **off-screen data**.

Use this option when you want to print **all** the data **in menus** like:

- **Timing and State Format Specifications**
- **State Trace Specifications**
- **State Listing**

What Happens during a Printout?

When you press select to start the printout, the I/O menu **pop-up** disappears and an advisory PRINT in progress appears in the top center of the display. While the data is transferred **to the** printer, the logic **analyzer's** keyboard deactivates. When the logic **analyzer has** completed **the** data transfer to the printer, the advisory disappears and the keyboard reactivates.

Don't worry! The Print in progress advisory won't appear in your printout.

Logic Analyzer Turn-on Check List

This appendix summarizes the steps you take to **turn** on the HP 1650B/51B logic analyzers. **The** details of the turn-on procedures are in **Chapter 1 of this booklet**.

1. Check the rear-panel line voltage indicator for **the** proper setting. **Change the setting if necessary.**
2. Make sure you **have** the proper **3-wire** grounded AC power cable.
3. Make sure the rear-panel **line** switch is **Off**.
4. **Connect** the power cable to the rear-panel line **connector** and a properly grounded power receptacle.
5. Make sure the yellow shipping disk is removed **from** the disk drive.
6. **Insert** the operating system disk in the disk drive.
7. Turn the logic analyzer on with the rear-panel line switch.

When the logic analyzer **completes** its self-tests, **it** then loads **the** operating **system** from the disk. When **the** operating system **has** been completely loaded, the System **Configuration** menu will be displayed.

Summary

Now that you have configured the RS-232C or HP-IB interface for your printer, you can make hardcopy printouts of anything that the logic analyzer displays. This is a valuable feature when you need to keep records of configurations and measurements.

Loading Demo Files from the Disk

To load the demo **files from** the disk, follow these **steps**:

1. Press the **I/O key on the front panel**
2. Place the cursor on *** Dii Operations** and press **SELECT**.

The disk drive indicator light will **come** on telling you the logic analyzer **is reading the disk**. **When the disk is read, the logic analyzer will show** you the directory of files on the disk.

3. Press the up/down **ROLL** key to activate the **roll** function.
4. Rotate the **KNOB** to place your **file selection** in the center of the **screen**. **The center of the screen has an arrow on each side of the display area pointing toward the center**.

When your **file selection** is **in** the center, it will be displayed in **bold type**.

5. Press the up/down **ROLL** key again to deactivate the file selection **function**.

Note



Check to see what is displayed in the field **in** the upper left of the menu. **If Load is displayed, skip steps 6 and 7.**

6. Place the cursor in the field in the **upper** left of the menu and press **SELECT**.
7. Place the cursor on **Load** and press **SELECT**. The **pop-up** will close and place **Load** in this field

Verify that your file selection is displayed in the box to the right of Load from file. If it is not, repeat step 4. If the correct file is displayed, continue to step 8.

8. Place the cursor on **Execute** and press SELECT.

The logic analyzer will load the file and display **Load operation complete**. You resume normal logic analyzer operation by selecting the menu key for the menu you want to see.

Herstellerbescheinigung

Hiermit wird bescheinigt, daß das Gerät/System

HP 1650B/HP 1651B

in Übereinstimmung mit den Bestimmungen von Postverfügung 1046/84 funkentstört ist.

Der Deutschen Bundespost wurde das Inverkehrbringen dieses Gerätes/Systems angezeigt und die Berechtigung zur Überprüfung der Serie auf Einhaltung der Bestimmungen ~~eingewährt~~.

Zusatzinformation für Meß- und Testgeräte

Werden Meß- und Testgeräte mit ungeschirmten Kabeln und/oder in offenen Meßaufbauten verwendet, so ist vom Betreiber sicherzustellen, daß die Funk-Entstörbestimmungen unter Betriebsbedingungen an seiner Grundstücksgrenze eingehalten werden.

Manufacturer's declaration

This is to certify that this product HP 1650B/HP 1651B meets the radio frequency interference requirements of directive Vfg. 1046/84. The German Bundespost has been notified that this equipment was put into circulation and was granted the right to check the product type for compliance with these requirements.

Additional Information for Test- and Measurement Equipment

Note: If test and **measurement equipment is operated with unshielded cables and/or used for measurements on open set-ups**, the user **must** insure that **under these operating conditions, the radio frequency interference limits are met at the border of his premises.**

Note: This declaration indicates compliance of this product with the German RFI specifications stated in the German Vfg. 1046/84 directive.

Timing Format Specification Menu

Introduction

This chapter describes the **Timing Format Specification menu** and all the **pop-up menus** that you will use on your timing analyzer. The purpose and function of each pop-up menu is explained in detail, and we have included many **illustrations** and **examples** to make the explanations clearer.

Accessing the Timing Format Menu

The **Timing Format Specification** menu can be accessed by pressing the **FORMAT** key on the front panel. If the **State Format Specification Menu** is displayed when you press the **FORMAT** key, you will have to switch **analyzers**. This is not a problem it merely indicates that the **last action** you performed in the **System Configuration** Menu was on the state **analyzer**.

Timing Format Specification Menu

The **Timing Format Specification** menu lets you **configure** the **timing** analyzer to group **channels** from your **microprocessor** into **labels** you assign for **your** measurements. You can set the **threshold** levels of the **poets assigned to the analyzer**, **assign labels and channels**, and **specify symbols**.

At power up, the logic **analyzer** is **configured** with a default setting. You can use this default setting to **make a test** measurement on the **system under test**. It can give you an idea of where to start your measurement. For an example of setting **up configurations** for the **Tii analyzer**, refer to the *Getting Started* Guide or "**Timing Analyzer Measurement Example**" in chapter 12 of this **manual**.

At power up the Timing Format Specification menu looks like that shown below:

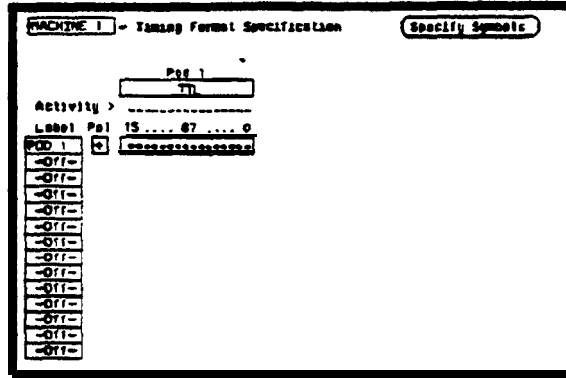


Figure 9-1. Timing Format Specification Menu

The Timing Format Specification menu for the HP 1651B is similar to that for the HP 1650B except that Pod 2 appears in the menu instead of Pod 5.

This menu shows only one pod assigned to each analyzer, which is the case at power up. Any number of pods can be assigned to one analyzer, from none to all five for the HP 1650B, and from none to two for the HP 1651B. In the timing Format Specification menu, only three pods appear at a time in the display. To view any pods that are off screen, press the left/right ROLL key and rotate the KNOB. The pods are always positioned so that the lowest numbered pod is on the right and the highest numbered pod is on the left.

Timing Format Specification Menu Fields

Five types of fields are present in the menu. They are:

- Label
- Polarity (Pol)
- Bit assignments
- Pod threshold
- Specify Symbols

A portion of the menu that is not a field is the Activity Indicators display. The indicators appear under the active bits of each pod, next to "Activity." When the logic analyzer is connected to your target system and the system is running, you will see 1 in the Activity Indicators display for each channel that has activity. These tell you that the signals on the channels are transitioning.

The fields in the Format menus are described in the following sections.

Label The label column contains 20 Label fields that you can define. Of the 20 labels, the logic analyzer displays only 14 in the Timing Format Specification menu at one time. To view the labels that are off screen, press the up/down ROLL key and rotate the KNOB. The labels scroll up and down. To deactivate the scrolling, press the ROLL key again.

To access one of the Label fields, place the cursor on the field and press SELECT. You will see a pop-up menu like that shown below.




Figure S-2 Label Pop-Up Menu

Turn Label On

Selecting this option turns the label on and gives it a default letter name. If you turned all the labels on they would be named A through T from top to bottom. When a label is turned on bit assignment fields for the label appear to the right of the label under the pods.

Modify Label

If you want to change the name of a label, or want to turn a label on and give it a specific name, you would select the **Modify label** option. When you do, an **Alpha Entry pop-up menu** appears. You can use the pop-up menu and the keypad on the front panel to name the label. A label name can be a maximum of six characters.

Turn Label Off

Selecting this option turns the label off. When a label is turned off, the bit assignments are saved by the logic analyzer. This gives you the option of turning the label back on and still having the bit assignments if you need them. The waveforms are also saved.

You can give the same name to a label in the state analyzer as in the timing analyzer without causing an error. The logic analyzer distinguishes between them. An example of this appears in "Using the Timing/State Analyzer" in chapter 7 of the *Getting Started Guide*.

Polarity (Pol)

Each label has a **polarity** assigned to it. The default for all the labels is **positive (+)** polarity. You can change the polarity of a label by placing the cursor on the polarity field and pressing **SELECT**. This toggles the polarity between **positive (+)** and **negative (-)**.

In the timing analyzer, negative polarity inverts the data.

Bit Assignment

The bit assignment fields allow you to assign MS (channels) to labels. Above each column of bit assignment fields is a line that tells you the bit numbers from 0 to 15, with the left bit numbered 15 and the right bit numbered 0. This line helps you know exactly which bits you are assigning.

The convention for bit assignment is:

- * (asterisk) indicates assigned bit
- . (period) indicates unassigned bit

At power up the 16 bits of Pod 1 are assigned to the timing analyzer and the 16 bits of Pod 5 are assigned to the state analyzer. To change a bit assignment configuration, place the cursor on a bit assignment field and press **SELECT**. You will see the following pop-up menu.




Figure 9-3. Bit **Assignment Pop-Up** Menu

Use the **KNOB** to move the cursor to an asterisk or a period and press **SELECT**. The bit assignment toggles to the opposite state of what it was before. When the bits (channels) are assigned as desired place the cursor on **Done** and press **SELECT**. This closes the pop-up and displays the new bit assignment.

Assigning one channel per label may be handy in some applications. This is illustrated in "Using the Timing/State Analyzer" in chapter 7 of the *Getting Started Guide* and chapter 12 of this manual. Also, you can assign a channel to more than one label, but this usually isn't desired.

Labels may have from 1 to 32 channels assigned to them. If you try to assign more than 32 channels to a label, the logic analyzer will beep, indicating an error, and a message will appear at the top of the screen telling you that 32 channels per label is the maximum.

Channels assigned to a label are numbered from right to left by the logic analyzer. The least significant assigned bit (LSB) on the far right is numbered 0, the next assigned bit is numbered 1, and so on. Since 32 channels can be assigned to one label at most, the highest number that can be given to a channel is 31. Although labels can contain split fields, assigned channels are always numbered consecutively within a label as shown in figure 9-4.

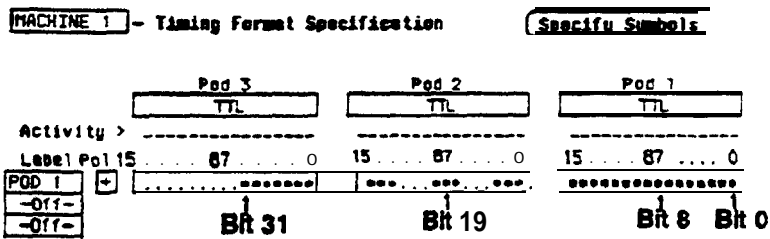


Figure 9-4. Numbering of Assigned Bits

Pod Threshold Each pod has a threshold level assigned to it. For the HP 1651B Logic Analyzer, threshold levels may be defined for Pods 1 and 2 individually. For the HP 1650B Logic Analyzer, threshold levels may be defined for Pods 1, 2 and 3 individually, and one threshold for Pods 4 and 5. It does not matter if Pods 4 and 5 are assigned to different analyzers. Changing the threshold of one will change the threshold of the other.

If you place the cursor on one of the pod threshold fields and press SELECT, you will see the following pop-up menu.




Figure 9-5. Pod Threshold Pop-Up Menu

TTL sets the threshold at + 1.6 volts, and ECL sets the threshold at -1.3 volts.

The User-defined option lets you set the threshold to a specific voltage between -9.9 V and + 9.9 V. If you select this option you will see a Numeric Entry pop-up menu as shown.

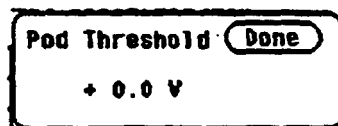


Figure 9-6. User-Defined Numeric Entry Pop-Up Menu

You can change the value in the pop-up either with the keypad on the front panel or with the KNOB, which you rotate until you get the desired voltage. When the correct voltage is displayed, press SELECT. The pop-up will close and your new threshold will be placed in the pod threshold field.

Specify Symbols Menu

The Specify Symbols field differs from the other fields in the Timing Format Specification menu in that it displays a complete menu instead of a pop-up.

The logic analyzer supplies Tii and State Symbol Tables in which you can define a mnemonic for a specific bit pattern of a label. When measurements are made by the timing analyzer, the mnemonic is displayed where the bit pattern occurs if the Symbol base is selected.

It is possible for you to specify up to 200 symbols in the logic analyzer. If you have only one of the internal analyzers on, all 200 symbols can be defined in it. If both analyzers are on, the 200 symbols are split between the two. For example, analyzer 1 may have 150, leaving 50 available for analyzer 2.

To access the Symbol Table in the Tii Format Specification menu, place the cursor on the Specify Symbols field and press SELECT. You will see a new menu as shown in figure 9-7. This is the default setting for the Symbol Table in both the timing and state analyzers.

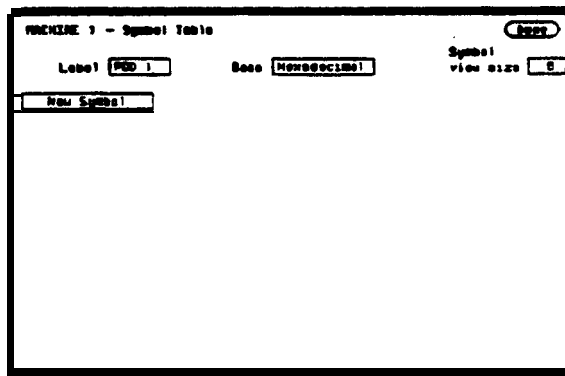


Figure 9-7. Symbol Table Menu

Specify Symbols Menu Fields

There are four fields in the Symbol Table menu. They are:

- Label
- Base
- Symbol view size
- Symbol name

Label The Label field identifies the label for which you are specifying symbols. If you select this field, you will get a pop-up that lists all the labels turned on for that analyzer.



Figure 9-8. Label Pop-Up Menu

Each label has a separate symbol table. This allows you to give the same name to symbols defined under different labels. In the Label pop-up select the label for which you wish to specify symbols.

Base The Base field tells you the numeric base in which the pattern will be specified. The base you choose here will affect the Find Pattern field of the Timing Trace Specification menu. This is covered later in this chapter.

To change the base, place the cursor on the Base field and press SELECT. You will see the following pop-up menu.





Figure 9-Q. Base Pop-Up Menu

If more than 20 channels are assigned to a label, the Binary option is not offered in the pop-up. The reason for this is that when a symbol is specified as a range, there is only enough room for 20 bits to be displayed on the screen.

Decide which base you want to work in and choose that option from the numeric Base pop-up menu.

If you choose the ASCII option, you can see what ASCII characters the patterns and ranges defined by your symbols represent. ASCII characters represented by the decimal numbers 0 to 127 (hex 00 to 7F) are offered on your logic analyzer. Specifying patterns and ranges for symbols is discussed in the next section.

Note 

You cannot specify a pattern or range when the base is ASCII. First define the pattern or range in one of the other bases, then switch to ASCII to see the ASCII characters.

Symbol View Size The Symbol view size field lets you specify how many characters of the symbol name will be displayed when the symbol is referenced in the Thing Trace Specification menu and the Thing Waveform menu. Selecting this field gives you the following pop-up.




Figure 9-10. Symbol View Size Pop-Up Menu

You can have the logic analyzer display from 3 to all 16 of the characters in the symbol name. For more information see "Timing Trace Specification Menu" in Chapter 10 and the "Timing Waveforms Menu" in Chapter 11.

Symbol Name When you first access the Symbol Table, there are no symbols specified. The symbol name field reads "New Symbol." If you select this field, you will see an Alpha Entry pop-up menu on the display. Use the pop-up menu and the keypad on the front panel to enter the name of your symbol. A maximum of 16 characters can be used in a symbol name. When you select the Done field in the Alpha Entry pop-up menu the name that appears in the symbol name field is assigned and two more fields appear in the display.



Figure 9-1 1. Symbol Defined as a **Pattern**

The first of these fields defines the symbol as either a **Pattern** or a **Range**. If you place the cursor on this field and press **SELECT**, it will toggle between **Pattern** and **Range**.

When the symbol is defined as a pattern, one field appears to specify what the pattern is. Selecting this field gives you a pop-up with which you can specify the pattern. Use the keypad and the **DON'T CARE** key on the front panel to enter the pattern. Be sure to enter the pattern in the numeric base that you specified in the **Base** field.



Figure 912 Specify **Pattern** Pop-Up

If the symbol is defined as a range, two fields appear in which you specify the upper and lower boundaries of the range.




Figure 813. Symbol Defined as a **Range**

Selecting either of these fields gives you a pop-up with which you can specify the boundary of the range.




Figure S-14. Specify **Range** Pop-Up

You can specify **ranges that** overlap or are nested within **each** other. Don't cares are not allowed.

To add more symbols to your symbol table, place the cursor on the last symbol **defined** and **press** SELECT. A pop-up **menu** appears as **shown**.




Figure 9-15. Symbol Pop-Up Menu

The first option in the pop-up is **Modify symbol**. If you select this option, you will see an **Alpha Entry** pop-up menu with which you can change the name of the symbol.

The second option in the pop-up is **Insert new symbol**. It allows you to specify another symbol. When you select it, you will see an **Alpha Entry** pop-up menu. Use the menu and the keypad on the front panel to enter the name of your new symbol. When you select **Done**, your new symbol will appear in the Symbol Table. The third option in the pop-up is **Delete symbol**. If you select this option, the symbol will be deleted from the Symbol Table.

Leaving the Symbol Table Menu

When you have specified all your symbols, you can leave the Symbol Table menu in one of two ways. One method is to place the cursor on the **Done** field and press **SELECT**. This puts you back in the **Format Specification** menu that you were in before entering the Symbol Table. The other method is to press the **FORMAT**, **TRACE**, or **DISPLAY** keys on the front panel to get you into the respective menu.

Timing Trace Specification Menu

introduction

This chapter describes Timing Trace Specification menu and all the pop-up menus that you will use on your timing analyzer. The purpose and function of each pop-up menu is explained in detail, and we have included many illustrations and examples to make the explanations clearer.

Accessing the Timing Trace Specification Menu

The Timing Trace Specification menu can be accessed by pressing the TRACE key on the front panel. If the State Trace Specification menu is displayed when you press the TRACE key, you will have to switch analyzers. This is not a problem, it merely indicates that the last action you performed in the System Configuration Menus was on the state analyzer.

Timing Trace Specification Menu

The Trace Specification menus allow you to configure the logic analyzer to capture only the data of interest in your measurement. In the timing analyzer you can configure the analyzer to trigger on specific patterns, edges, or glitches. The Timing Trace Specification menu lets you specify the trigger point for the logic analyzer to start capturing data and the manner in which the analyzer will capture data. You configure the timing analyzer to find a pattern first and then a transition in the signal or signals.

At power up, the logic analyzer is configured with a default setting. You can use this default setting to make a test measurement on the system under test. It can give you an idea of where to start your measurement. For an example on setting up configurations for the Timing analyzer, refer to the *Getting Started Guide* or "Timing Analyzer Measurement Example" in Chapter 12 of this manual.

At power up the Timing Trace menu looks like that shown below.

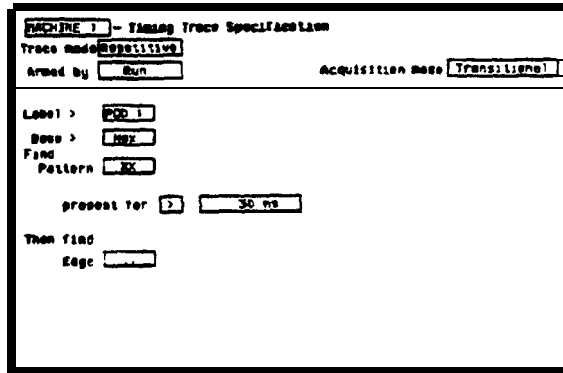


Figure 10-1. Timing Trace Specification Menu

The menu is divided into two sections by a horizontal line. The top section contains the fields that you use to specify the data acquisition. The bottom section contains the fields for setting the trigger point.

Timing Trace Specification Menu Fields

The fields in the Timing Trace Specification menu are:

- Trace mode
- Armed by
- Acquisition mode
- Level
- Base
- Find Pattern
- Pattern Duration (present for _____)
- Then find Edge

These are described in the following sections.

Trace Mode With the Trace Mode field you specify the mode in which the timing analyzer will trace. You have two choices for Trace mode: Single and Repetitive. If you place the cursor on the field and press SELECT, the field toggles from one mode to the other.

Single Trace mode acquires data once per trace. Repetitive Trace mode repeats single acquisitions until the STOP key on the front panel is pressed, or if Stop measurement has been selected and the stop measurement condition has been met.

If both analyzers are on, only one trace mode can be specified. Specifying one trace mode for one analyzer sets the same trace mode for the other analyzer.

Armed By The Armed by field lets you specify how your timing analyzer is to be armed. The analyzer can be armed by the RUN key, the other analyzer, or an external instrument through the BNC Input port.

When you select the Armed by field, a pop-up menu appears like that shown below. Use this menu to select the arming option for your analyzer.

Run
BNC Input
MACHINE 2

Figure10-2. Armed ByPop-Up Menu

Acquisition Mode The Acquisition mode field allows you to specify the mode in which you want the timing analyzer to acquire data. You are given two choices for the mode of acquisition: Transitional and Glitch . If you place the cursor on this field and press SELECT, the field toggles from one mode to the other.

Transitional Acquisition Mode

When the logic analyzer is operating in the Transitional Acquisition mode, it samples the data at regular intervals, but it stores data in memory only on transitions in the signals. A time tag that is stored with each sample allows reconstruction of the samples in the Time Waveforms display.

Transitional timing always samples at a rate of 100 MHz (10 ns/sample). This provides maximum timing resolution even in records that span long time windows. Time covered by a full memory acquisition varies with the number of pattern changes in the data. If there are many transitions, the data may end prior to the time window desired because the memory is full. However, a prestore qualification in your logic analyzer insures that data will be captured and displayed between the left side of the screen and the trigger point.

Figure 10-3 illustrates Transitional acquisition, comparing it to Traditional -

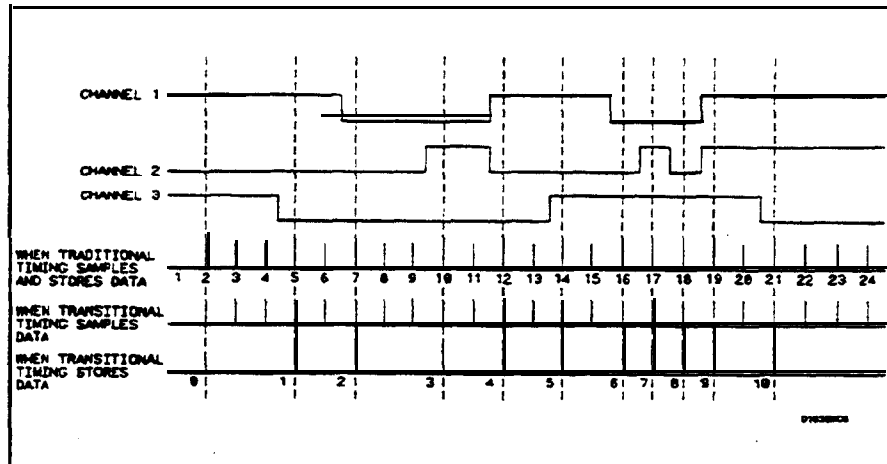


Figure 10-3. Transitional vs. Traditional Acquisition

Traditional timing samples and stores data at regular intervals. Transitional timing samples data at regular intervals but stores a sample only when there has been a transition on one or more of the channels. This makes it possible for Transitional timing to store more information in the same amount of memory.

Glitch Acquisition Mode

A glitch is defined as any transition that crosses logic threshold more than once between samples. It can be caused by capacitive coupling between traces, by power supply ripples, or a number of other events. Since a glitch can cause major problems in your system, you can use the Glitch mode to find it.

Your logic analyzer has the capability of triggering on a glitch and capturing all the data that occurred before it. The glitch must have a width of at least 5 ns at threshold in order for the analyzer to detect it.

If you want your timing analyzer to trigger on a glitch in the data set the Acquisition mode to Glitch. This causes several changes in the analyzer. One change is that a field for glitch detection in each label is added to the Timing Trace Specification menu, as shown:

Then find
Edge
or
Glitch

Figure 10-4. Glitch Specification Field

With these glitch detection fields you specify on which channel or channels you want the analyzer to look for a glitch. These fields are discussed in more detail in "Then Find Edge" later in this chapter.

Glitch Acquisition mode causes the storage memory to be cut in half from 1k to 512. Half the memory (512) is allocated for storing the data sample, and the other half for storing the second transition of a glitch in a sample. Every sample is stored.

The sample rate varies from 20 Hz to 50 MHz (50 ns/sample to 20 ns/sample) and is automatically selected by the timing analyzer to insure complete data in the window of interest.

When your timing analyzer triggers on a glitch and displays the data, the glitch appears in the waveform display as shown below.

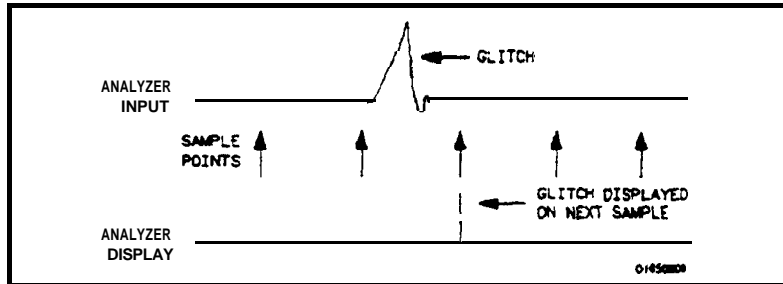


Figure 10-5. Glitch In timing Waveform

Label The Label fields contain the labels that you define in the Timing Format Specification menu. If there are more labels than can fit on screen, use the left/right ROLL key and the KNOB to view those that are not displayed.

Base The Base fields allow you to specify the numeric base in which you want to define a pattern for a label. The Base fields also let you use a symbol that was specified in the Timing Symbol Table for the pattern. Each label has its own base defined separately from the other labels. If you select one of the Base fields, you will see the following pop-up menu. Decide which base you want to define your pattern in and select that option.




Figure 10-6. Base Pop-up Menu

One of the options in the Base pop-up is ASCII . It allows you to see characters that are represented by the pattern you specified in the Find Pattern field.

```
Label > [ POD 1 ]
Base > [ ASCII ]
Find
Pattern [ * ]
```

Figure 10-7. ASCII Defined as Numeric Base

Notice in the figure above that the Find Pattern field is no longer a selectable field when the base is ASCII . You cannot specify ASCII characters directly. You must specify a pattern in one of the other bases; then you can switch the base to ASCII and see what characters the pattern represents.

The Symbol option in the Base pop-up allows you to use a symbol that has been specified in the Timing Symbol Tables as a pattern or specify absolute and enter another pattern. You specify the symbol you want to use in the Find Pattern field.

Find Pattern With the Find Pattern fields, you configure your timing analyzer to look for a certain pattern in the data. Each label has its own pattern field that you use to specify a pattern for that label.

During a run, the logic analyzer looks for a pattern in your data which is the logical AND of all the labels' patterns. That is, it looks for a simultaneous occurrence of the specified patterns. When it finds the pattern, it triggers at the point that you specified in the Then find Edge fields. See "Then Find Edge" later in this chapter for more information about edge triggering.

You select a Find Pattern field with one of two methods. The first method is to place the cursor on the Find Pattern field and press SELECT. The second method is to place the cursor on the Find Pattern field and press one of the alphanumeric keys on the front-panel keypad. Both methods give you a pop-up similar to that shown in figure 10-8.

Specify Pattern:

2425

Figure 10-8. Specify Pattern Pop-Up for Find Pattern

The pop-up will vary depending on the base you choose and the number of channels you assign to that label. If you press a key on the keypad to open the pop-up, the character on the key is placed in the first location of the pattern.

Enter your pattern in the pop-up and press SELECT. The pattern appears under the label in the Find Pattern field.

As mentioned previously in "Base", if you specify ASCII as the base for the label, you won't be able to enter a pattern. You must specify one of the other numeric bases to enter the pattern. Then you can switch the base to ASCII and see what ASCII characters the pattern represents. If you choose Symbols in the Base field, you can use one of the symbols specified in the Timing Symbol Tables as the pattern. The Find Pattern field looks similar to that below:

```
Label >  [ POD 1 ]
Base >   [ Symbol ]
Find
Pattern [ absolute 2425 ]
```

Figure 10-9. Symbol Defined in Base Fii

If you select this field you get a pop-up similar to that shown:

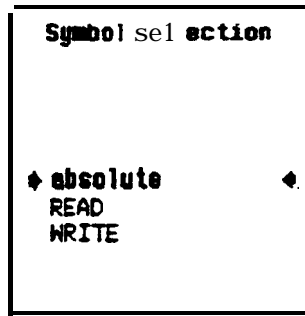


Figure 10-10. Symbol Selection Pop-Up for Find Pattern

The pop-up lists all the symbols defined for that label. It also contains an option "absolute xxx." Choosing this option gives you another pop-up with which you specify a pattern not given by one of your symbols.

To select an option from the pop-up, use the KNOB to scroll the symbols up and down until the desired symbol is between the two arrows. Press SELECT. The symbol name appears in the Find Pattern field under the label.

When you specify symbols in the Timing Symbol Tables, you also specify the number of characters in the symbol name that are to be displayed. If you specify only three characters of a symbol name in the Symbol menu, only REA of READ and WRI of WRITE would be displayed in the Find Pattern Field. In addition, only the first three letters of "absolute" would be displayed.

Pattern Duration
(present for) _____

There are two fields with which you specify the Pattern Duration. They are located next to present for _____ in the Timing Trace Specification menu. You use these fields to tell the timing analyzer to trigger before or after the specified pattern has occurred for a given length of time

The first field can be set to " > " (greater than) or " < " (less than). If you place the cursor on this field and press SELECT, it toggles between > and <. The second field specifies the duration of the pattern. If you select > in the first field, you can set the duration to a value between 30 ns and 10 ms. If you select < in the first field, you can set the duration to a value between 40 ns and 10 ms. If you attempt to set the duration to a value outside the given range, the analyzer will automatically set it to the nearest hit.

To change the value of the pattern duration, place the cursor on the second field and either press SELECT to get a pop-up menu, or just press one of the numeric keys on the front-panel keypad. Both methods give you a Numeric Entry pop-up similar to that shown.

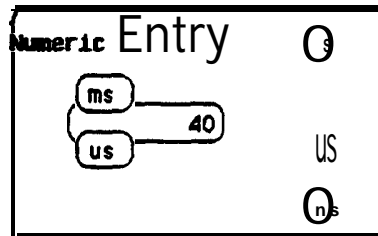


Figure 10-11. Pattern Duration (present for) Pop-Up

With the front-panel keypad enter the desired pattern duration. Use the KNOB to place the cursor on the correct timing units, then press SELECT. Your value for Pattern Duration will appear in the field.

Note

If you press a key on the keypad to open the pop-up, the number that you pressed will appear in the entry field replacing the previous value. To restore the original value press the CLEAR ENTRY key.

As an example, suppose you configure the present for ____ field as shown:

present for I >

Figure 10-12. Example of Pattern Duration (Greater Than)

This configuration tells the timing analyzer to look for the pattern you specified that occurs for a period of time greater than 50 ns. Once the timing analyzer has found the pattern, it can look for the trigger.

Choosing < (less than) forces glitch and edge triggering off, and the timing analyzer triggers immediately at the end of the pattern that meets the duration requirements. The fields with which you specify edges and glitches don't appear in t&e menu. For instance, if you configure the present for ____ field as shown:

present for I <

Figure 10-13. Example of Pattern Duration (Less Than)

The analyzer will trigger when it sees the pattern you specified that occurs for a period less than 100 ns. The pattern must also be valid for at least 20 ns.

Then Find Edge

With the Then find Edge fields you can specify the edges (transitions) of the data on which your timing analyzer triggers. You can specify a positive edge, a negative edge, or either edge. Each label has its own edge trigger specification field so that you can specify an edge on any channel.

When you specify an edge on more than one channel, the timing analyzer logically ORs them together to look for the trigger point. That is, it triggers when it sees any one of the edges you specified. It also ANDs the edges with the pattern you specified in the Find Pattern fields. The logic analyzer triggers on an edge following the valid duration of the pattern while the pattern is still present. To specify an edge, place the cursor on one of the Then find Edge fields and press SELECT. You will see a pop-up similar to that shown in the following figure.




Figure 10-14. Specify Edge Pop-Up for Then Find Edge

Your pop-up may look different than this depending on the number of channels you assigned to the label. Each period in the pop-up indicates

To specify a negative edge, place the cursor on one of the periods in the pop-up and press SELECT once. The period changes to ↓, as shown:



Figure 10-15. Negative Edge Specified

To specify a positive edge, place the cursor on one of the periods and press SELECT twice. The period changes to ↑, as shown:




Figure 10-16. Positive Edge Specified

If you want the analyzer to trigger on either a positive or a negative edge, place the cursor on a period and press SELECT three times. The period changes to ↓↑, as shown:





Figure 10-17. Either Edge Specified

If you want to delete an edge specification, place the cursor on the arrow for that channel and press SELECT until you see a period. To clear an entire label, press the CLEAR ENTRY key on the front panel.

When you have finished specifying edges, place the cursor on the Done field and press SELECT to close the pop-up.

Note 

If you are not in Binary base, you will see dollar signs (\$\$..) in the Then find Edge field when you close the pop-up. These indicate that edges have been specified; however, the logic analyzer can't display them correctly unless you have selected Binary for the base.

Glitch Triggering. When you set the Acquisition mode on Glitch a glitch detection field for each label is added to the screen. These fields allow you to specify glitch triggering on your timing analyzer. Selecting one of these fields brings up the following pop-up menu.




Figure 10-18. Specify Glitch Pop-Up for Then Find Glitch

Your pop-up may look different depending on the number of channels you have assigned to the label. Each period indicates that the channel has not been specified for glitch triggering.

To specify a channel for glitch triggering, place the cursor on one of the periods and press SELECT. The period is replaced with an asterisk, indicating that the logic analyzer will trigger on a glitch on this channel.



Figure 10-19. Glitches Specified

If you want to delete a glitch specification, place the cursor on the asterisk and press SELECT. The asterisk is replaced with a period.

Note



If you are not in Binary base, you will see dollar signs (\$\$.) in the Glitch field when you close the pop-up. This indicates that glitches have been specified; however, the logic analyzer can't display them correctly unless you have selected Binary for the base.

When more than one glitch has been specified, the logic analyzer logically ORs them together. In addition, the logic analyzer ORs the glitch specifications with the edge specifications, then ANDs the result with the pattern you specified in the Find Pattern fields in order to find the trigger point. A boolean expression illustrating this is:

$(\text{glitch} + \text{glitch} + \text{edge} + \text{edge}) * \text{pattern}$

Note



If you select c (less than) in the present field, edge and glitch triggering are turned off. The Then find Edge or Glitch field no longer appears on the screen. The logic analyzer then triggers only on the pattern specified in the Find Pattern fields.

Timing Waveforms Menu

Introduction

The **Timing Waveforms menu** is the display **menu** of the timing analyzer. This chapter **describes** the **Timing Waveforms menu** and how to **interpret** it. It also tells you how to use the fields to manipulate the displayed data so you can find your measurement answers.

There are two different areas of the timing waveforms display: the menu area and the waveforms area. The menu area is in the top one-fourth of the screen and the waveforms area is the bottom three-fourths of the screen.

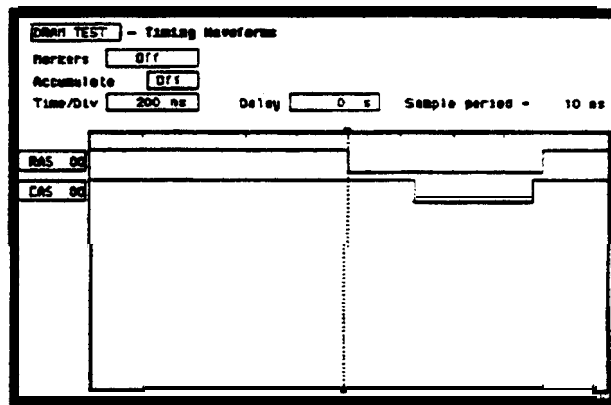


Figure 11-1. Timing **Waveforms Menu**

The waveforms area displays the data that the timing analyzer acquires. The data is displayed in a format similar to an oscilloscope with the horizontal axis representing time and the vertical axis representing amplitude. The basic differences between an oscilloscope display and the timing waveforms display are: in the timing waveforms display the vertical axis only displays highs (above threshold) and lows (below threshold). Also, the waveform lows are represented by a thicker line for easy differentiation.

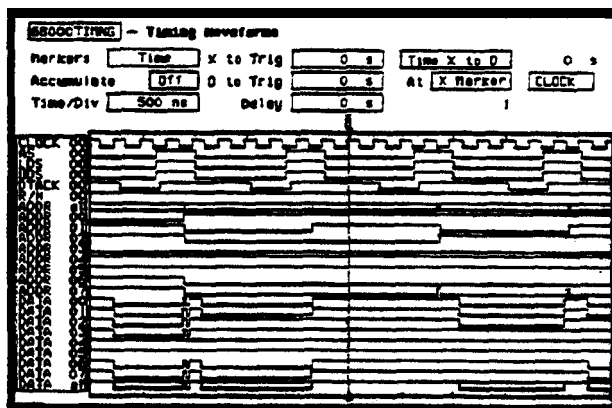


Figure 11-2. Timing Waveforms Menu with 24 Waveforms

Accessing the Timing Waveforms Menu

The Timing Waveforms Menu is accessed by the pressing the DISPLAY key on the front panel when the timing analyzer is on. It will automatically be displayed when you press RUN.

Timing Waveforms Menu Fields

The menu area contains fields that allow you to change the display parameters, place markers, and display waveform measurement parameters.




Figure 11-3. Timing Waveforms Menu Fields

Markers The Markers field allows you to specify how the X and O markers will be positioned on the timing data. The options are:

- Off
- Time
- Patterns
- Statistics
- Markers Off/Sample Period

When the markers are off they are not visible and the sample period is displayed. In transitional timing mode, the sample period will always be 10 ns. In Glitch, the sample period is controlled by the Time/Div setting and can be monitored by turning the markers off.

Note

The sample period displayed is the sample period of the last acquisition. If you change the Time/Div setting, you must press RUN to initiate another acquisition before the sample period is updated.

Although the markers are off, the logic analyzer still performs statistics, so if you have specified a stop measurement condition the measurement will stop if the pattern specified for the markers is found.




Figure 11-4. Markers Off

Markers Time When the markers are set CO Time, you can place the markers on the waveforms at events of interest and the logic analyzer will tell you:

- Time X to Trig(ger)
- Time O to Trig(ger)
- Time X to O

To position the markers, move the cursor to the field of the marker you wish to position and press SELECT. A pop-up will appear showing the current time for that marker. Either rotate the KNOB or enter a numeric value from the keypad to change the position of that marker. Pressing SELECT when you are finished positions the marker and closes the pop-up.

When the cursor is on either the X to Trig or O to Trig fields, you can also enter a value directly from the keypad without pressing SELECT.




Figure 11-5. Markers Time

The Time X to O field will change according to the position of the X and O markers. If you place the cursor on the Time X to O field and press SELECT, another pop-up will appear showing you all three times: X to Trigger, O to Trigger, and Time X to O.




Figure 11-6. Time X to O Pop-up

If you rotate the KNOB while this pop-up is open, both X and O markers will move, but the relative placement between them will not change.

Markers Patterns

When the markers are set to patterns, you can specify the patterns on which the logic analyzer will place the markers. You can also specify how many occurrences of each marker pattern the logic analyzer looks for. This use of the markers allows you to find time between specific patterns in the acquired data.

DRAM TEST - Timing Waveforms Specify Patterns

Markers Find x-pattern from Trigger

Accumulate Find o-pattern from

Time/Div Delay Time X to O

Figure 11-7. Markers Patterns

Patterns for each marker (X and O) can be specified. Patterns can be specified for both markers in each label. The logic analyzer searches for the logical "and" of patterns for all labels even though only one label can be displayed at a time. You can also specify whether the marker is placed on the pattern at the beginning of its occurrence (entering) or at the end of its occurrence (leaving) as shown in figure 11-8.

Marker Patterns Done

Label Base

X Marker > pattern

O Marker > pattern

Stop measurement:

Store exception to disk: File name


File description

Figure 11-8. Marker Patterns pop-up menu

Stop Measurement. Another feature of markers set to patterns is the Stop measurement when Time X-O _____. The options are: Less than, Greater than, In range, Not in range

With this feature you can use the logic analyzer to look for a specified time or range of time between the marked patterns and have it stop acquiring data when it sees this time between markers. (The X marker must precede the O marker.)

Also available is **Store exception to disk** which allows you to specify a file on the disk that exceptions can be stored in. The default filename is **EXCEPTION**.

Note 

The upper and lower range boundaries must **not** be the same value. For example, if you want to stop a measurement when the X and O markers are in range of 200 ns, you should set the range values to 190 ns and 210 ns. This eliminates erroneous measurement termination.

Markers Statistics

When statistics are **specified** for **markers**, the logic analyzer will display the:

- **Number of total runs**
- **Number of valid runs** (runs where **markers** were able to be placed on specified patterns)
- **Minimum time between the X and O markers**
- **Maximum time between the X and O markers**
- **Average time between the X and O markers**

Statistics are based on the time between markers which are placed on specific patterns. If a marker pattern is not specified, the marker will be placed on the trigger point by the logic analyzer. In this case the statistical measurement will be the time from the trigger to the specified marker. How the statistics will be updated depends on the timing trace mode (repetitive or single).

In repetitive, statistics will be updated each time a valid run occurs until you press STOP. When you press RUN after STOP, the statistics will be cleared and will restart from zero.

In single, each time you press RUN an additional valid run will be added to the data and the statistics will be updated. This will continue unless you change the placement of the X and O markers between runs.

Accumulate Mode

Accumulate mode is **selected** by toggling the **Accumulate ON/OFF** field in the **Timing Waveforms menu**. When accumulate is **on**, the timing analyzer displays the data from a current acquisition on top of the previously acquired data

When the old data is cleared depends on whether the trace mode is in single or repetitive. In single, new data will be displayed on top of the old each time RUN is selected as long as you stay in the Timing Waveforms menu between runs. Leaving the Timing Waveforms menu always clears the accumulated data. In repetitive mode, data is cleared from the screen only when you start a run after stopping acquisition with the STOP key.

AT _____
 Marker _____

The At X (or O) Marker _____ fields allow you to select either the X or O markers. You can place these markers on the waveforms of any label and have the logic analyzer tell you what the pattern is. For example, in the timing waveforms display (figure 6-8) the number 35 to the right of the Delay _____ field is the pattern in hexadecimal that is marked by the O marker. The base of the displayed field is determined by the base of the specified label you selected in the Timing Trace menu.

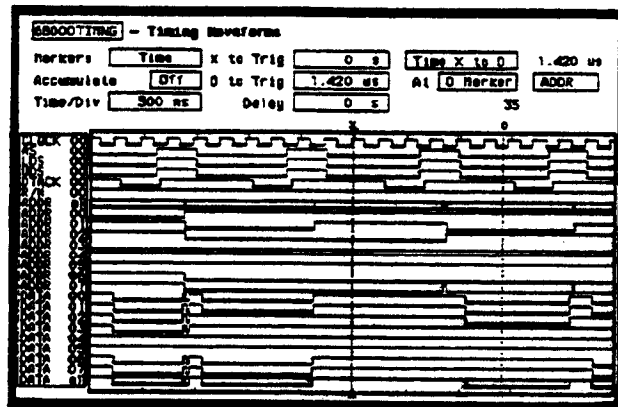


Figure 11-S. At 0 Marker ADDR fields

This display tells you that 35H is the pattern on the address label lines where the O marker is located.

You can toggle the At _____ Marker field between the X and O markers.

The next field to the right of the At ____ Marker field will pop up when selected and show you all the labels assigned to the timing analyzer as shown below.

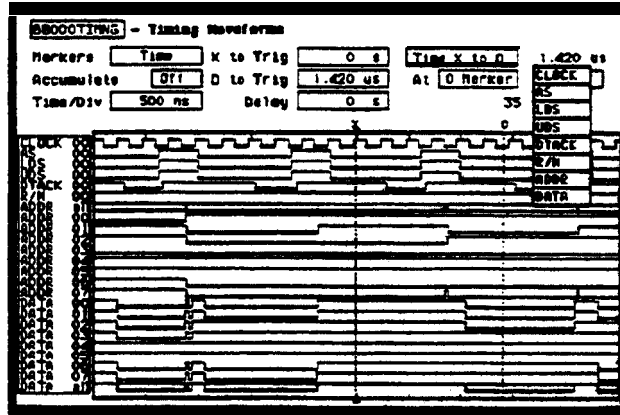


Figure 11-10. Label Option Pop-up

Time/Div (time per division) Field

The time per division field allows you to change the width of the time window of the Timing Waveforms menu.

When the pop-up is open you can change the time per division by rotating the KNOB or entering a numeric value from the keypad. When you rotate the KNOB, the time per division increments or decrements in 1-2-5 sequence from 10 ns/div to 50 ms/div.

Note 

Sample period is fixed at 10 ns in the Transitional acquisition mode.

When you enter a value from the keypad, the time per division does not have to be a 1-2-5 sequence.

Note 

In Glitch mode, changing the Time/Div setting changes the sample period for the next run. To view the sample period after the next run, turn the markers off if they are on and press RUN.

Delay Field

The Delay field allows you to enter a delay. The delay can be either positive or negative. Delay allows you to place the time window (selected by Time/Div) of the acquired data at center screen.

The inverted triangle in the horizontal center of the waveforms area of the display represents trigger + delay. The vertical dotted line represents the trigger point (see figure 6-10).

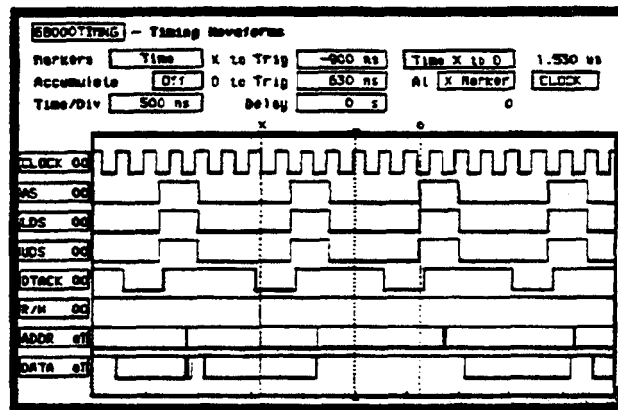


Figure 11-11. Trigger and Trace Points

If you want to trace after the trigger point, enter a positive delay. If you want to trace before the trigger-point (similar to negative time) enter a negative delay. The logic analyzer is capable of maximum delays of -2500 seconds to +2500 seconds. In Transitional mode the maximum delay is determined by the number of transitions of the incoming data. Data may not be displayed at all settings of Time/Div and Delay.

In Glitch mode the maximum delay is 25 seconds, which is controlled by memory and sample period (512 x 50ms). The sample rate is also dependent on the delay setting. It is represented by the following formula:

if delay < 20 ns

Hwdelay = 20 ns (this is an instrument constant)

if delay > 10 ms

Hwdelay = 10 ms

else Hwdelay = delay (delay setting in timing waveforms menu)

Sample period = larger of:

Time/Div ÷ 25 or

absolute value [(delay - Hwdelay) ÷ 256]

If sample period > 50 ms

Then sample period = 50 ms

Timing Analyzer Measurement Example

Introduction

In this chapter you will learn how to use the timing analyzer by setting up the logic analyzer to make a simple measurement. We give you the measurement results as actually measured by the logic analyzer, since you may not have the same circuit available.

The exercise in this chapter is organized in a task format. The tasks are ordered in the same way you will most likely use them once you become an experienced user. The steps in this format are both numbered and lettered. The numbered steps state the step objective. The lettered steps explain how to accomplish each step objective. There is also an example of each menu after it has been properly set up.

How you use the steps depends on how much you remember from chapters 1 through 4 of the *Getting Started Guide*. If you can set up each menu by just looking at the menu picture, go ahead and do so. If you need a reminder of what steps you need to perform, follow the numbered steps. If you still need more information about "how," use the lettered steps.

When you have finished configuring the logic analyzer for this exercise, you can load a file from the operating system disc. This file configures the logic analyzer the same way it is configured for this exercise. It also loads the same data acquired for this exercise so you can see what it looks like on screen.

In order to learn how to configure the logic analyzer, we recommend that you follow the exercise to "Acquiring the Data" before loading the file from the disc.

You can also compare your configuration with the one on the disc by printing it (if you have a printer) or making notes before you load the file.

Problem Solving with the Timing Analyzer

In this exercise, assume you are designing a dynamic RAM memory (DRAM) controller and you must verify the timing of the row address strobe (RAS) and the column address strobe (CAS). You are using a 4116 dynamic RAM and the data book specifies that the minimum time from when LRAS is asserted (goes low) to when LCAS is no longer asserted (goes high) is 250 ns. You could use an oscilloscope but you have an HP 1650A/51A on your bench. Since the timing analyzer will do just fine when you don't need voltage parametrics you decide to go ahead and use the logic analyzer.

What Am I Going to Measure?

After configuring the logic analyzer and hooking it up to your circuit under test, you will be measuring the time (x) from when the RAS goes low to when the CAS goes high, as shown below.

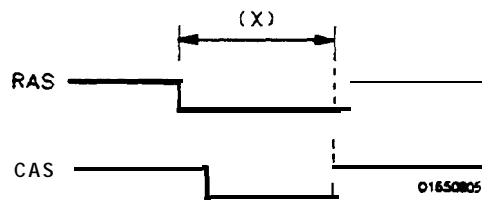


Figure 12-1. RAS and CAS Signals

How Do I Configure the Logic Analyzer?

In order to make this timing measurement, you must configure the logic analyzer as a timing analyzer. By following these steps you will configure Analyzer 1 as the timing analyzer.

If you are in the System Configuration menu you are in the right place to get started and you can start with step 2; otherwise, start with step 1.

1. Using the field in the upper left corner of the display, get the System Configuration menu on screen.
 - a. Place the cursor on the field in the upper left corner of the display and press SELECT.
 - b. Place the cursor on System and press SELECT.
2. In the System Configuration menu, change Analyzer 1 type to Timing. If analyzer 1 is already a timing analyzer, go on to step 3.
 - a. Place the cursor on the Type: ___ field and press SELECT.
 - b. Place the cursor on Timing and press SELECT.

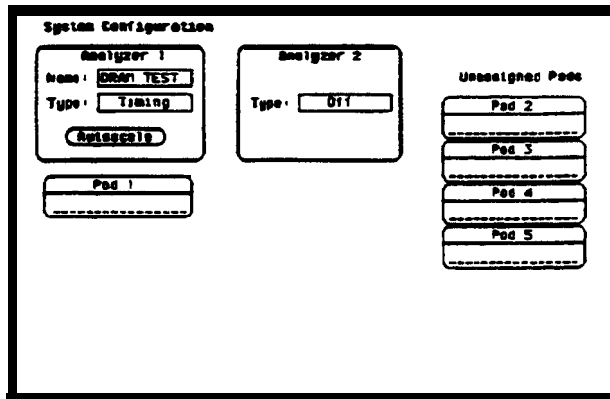


Figure 12-2. System Configuration Menu

3. Name Analyzer 1 "DRAM TEST" (optional)

- a. Place the cursor on the Name: ____ field of Analyzer 1 and press SELECT.
- b. With the Alpha Entry pop-up, change the name to "DRAM TEST" (see "How to Enter Alpha Data" in chapter 3 if you need a reminder).

4. Assign pod 1 to the timing analyzer.

- a. Place the cursor on the Pod 1 field and press SELECT.
- b. In the Pod 1 pop-up, place the cursor on Analyzer 1 and press SELECT.

Connecting the Probes

At this point, if you had a target system with a 4116 DRAM memory IC, you would connect the logic analyzer to your system.

Since you will be assigning Pod 1 bit 0 to the RAS label, you hook Pod 1 bit 0 to the memory IC pin connected to the RAS signal. You hook Pod 1 bit 1 to the IC pin connected to the CAS signal.

Activity Indicators

When the logic analyzer is connected and your target system is running, you will see **1** at the right-most end (least significant bits) of the Pod 1 field in the System Configuration menu. This indicates the RAS and CAS signals are transitioning.

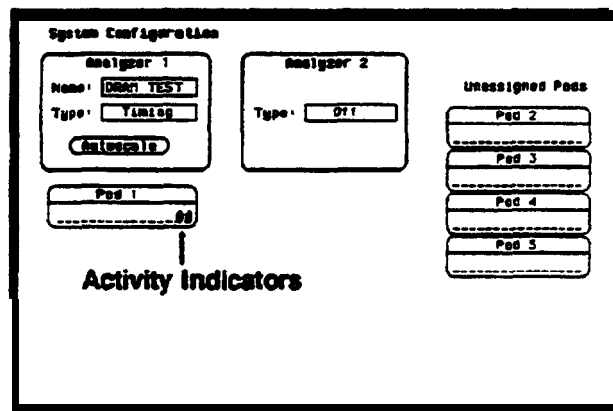


Figure 12-3. Activity Indicators

Configuring the Timing Analyzer

Now that you have configured the system, you are ready to configure the timing analyzer. You will be:

- Creating two names (labels) for the input signals
- Assigning the channels connected to the input signals
- Specifying a trigger condition

1. Display the TIMING FORMAT SPECIFICATION menu.

- a. Press the FORMAT key on the front panel.

2. Name two labels, one RAS and one CAS.

- a. Place the cursor on the top field in the label column and press SELECT.
- b. Place the cursor on Modify label and press SELECT .

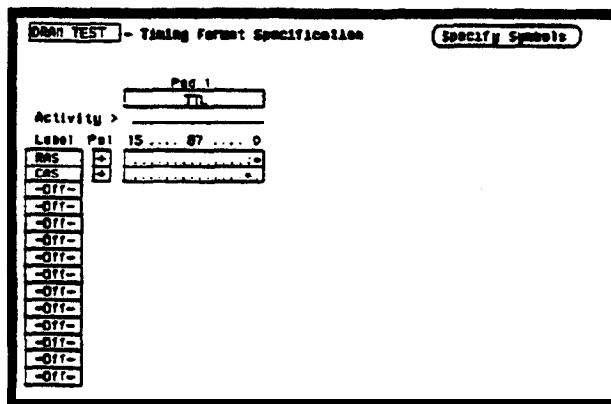


Figure 12-4. Timing Format Specification Menu

- c. With the Alpha Entry pop-up, change the name of the label to RAS.
 - d. Name the second label CAS by repeating steps a through c.
 3. Assign the channels connected to the input signals (Pod 1 bits 0 and 1) to the labels RAS and CAS respectively.
 - a. Place the cursor on the bit assignment field below Pod 1 and to the right of RAS and press SELECT.
 - b. Any combination of bits may be assigned to this pod; however, you will want only bit 0 assigned to the RAS label. The easiest way to assign bits is to press the CLEAR ENTRY key to unassign any assigned bits before you start.
 - c. Place the cursor on the period under the 0 in the bit assignment pop-up and press SELECT . This will place an asterisk in the pop-up for bit 0 indicating Pod 1 bit 0 is now assigned to the RAS label. Place cursor on Done and press SELECT to close the pop-up.
 - d. Assign Pod 1 bit 1 to the CAS label by moving the cursor to bit 1 and pressing SELECT.

Specifying a Trigger Condition

To capture the data and then place the data of interest in the center of the display of the TIMING WAVEFORMS menu, you need to tell the logic analyzer when to trigger. Since the first event of interest is when the LRAS is asserted (negative-going edge of RAS), you need to tell the logic analyzer to trigger on a negative-going edge of the RAS signal.

1. Select the TIMING TRACE menu by pressing the TRACE key.
2. Set the trigger so that the logic analyzer triggers on the negative-going edge of the RAS.
 - a. Place the cursor on the Then find Edge field under the label RAS, then press SELECT.
 - b. Place the cursor on the . (period) in the pop-up and press SELECT once. Pressing SELECT once in this pop-up changes a period to ↓ which indicates a negative-going edge.
 - c. Place the cursor on Done and press SELECT. The pop-up closes and a \$ will be located in this field. The \$ indicates an edge has been specified even though it can't be shown in the HEX base.

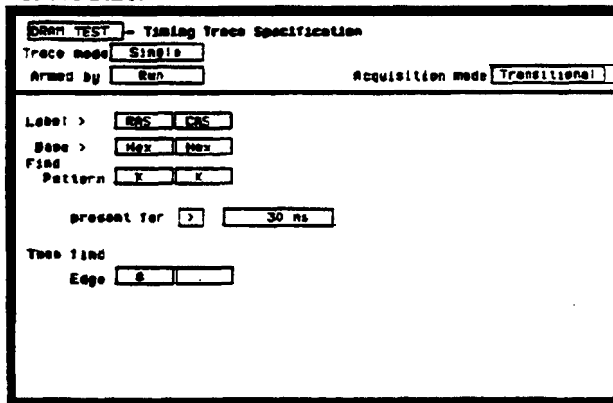


Figure 12-5. Trigger Edge Specified

Acquiring the Data

Now that you have configured and connected the logic analyzer, you acquire the data for your measurement by pressing the RUN key. The logic analyzer will look for a negative edge on the RAS signal and trigger if it sees one. When it triggers, the display switches to the TIMING WAVEFORMS menu.

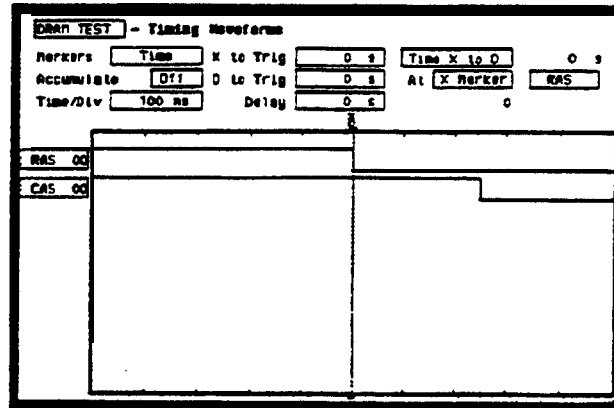


Figure 12-6. Timing Waveforms Menu

The RAS label shows you the RAS signal and the CAS label shows you the CAS signal. Notice the RAS signal goes low at or near the center of the waveform display area (horizontal center).

Now is the time to load the timing measurement demo file from the disc if you wish. The file name is TIMINGDEMO. Refer to "Load Operation" in chapter 6 if you need a reminder on how to load a file.

The Timing Waveforms Menu

The Timing Waveforms menu differs from the other menus you have used so far in this exercise. Besides displaying the acquired data, it has menu fields that you use to change the way the acquired data is displayed and fields that give you timing answers. Before you can use this menu to find answers, you need to know some of the special symbols and their functions. The symbols are:

- The X and O
- The ▼
- The vertical dotted line

The X and O The X and O are markers you use to find your answer. You place them on the points of interest on your waveforms, and the logic analyzer displays the time between the markers. The X and O markers will be in the center of the display when X to trig (ger) and O to trig (ger) are both 0.000 s (see example below).

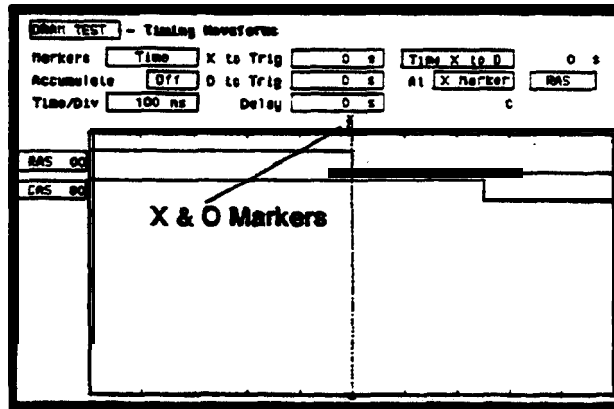


Figure 12-7. X & O Markers

The ▼

The ▼ (inverted triangle) indicates the trace point. Remember, trace point = trigger + delay. Since delay in this example is 0.000 s, you will see the negative-going edge of the RAS signal at center screen under the ▼.

The Vertical Dotted Line

The vertical dotted line indicates the trigger point you specified in the Timing Trace Specification menu. The vertical dotted line is at center screen under the inverted triangle and is superimposed on the negative-going edge of the RAS signal.

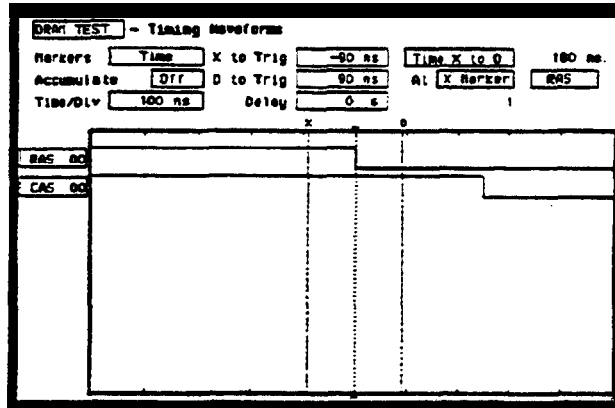


Figure 12-8. Inverted Triangle & Vertical Dotted Line

Configuring the Display

Now that you have acquired the RAS and CAS waveforms, you need to configure the Timing Waveforms menu for best resolution and to obtain your answer.

Display Resolution

You get the best resolution by changing the Time/Div to a value that displays one negative-going edge of both the RAS and CAS waveforms. Set the Time/Div by following these steps.



Figure 12-9. RAS and CAS Signals

1. Place the cursor on Time/Div and press SELECT . The pop-up appears, showing you the current setting.
2. While the pop-up is present, rotate the KNOB until your waveform shows you only one negative-going edge of the RAS waveform and one positive-going edge of the CAS waveform (see above). In this example 200 ns is best.

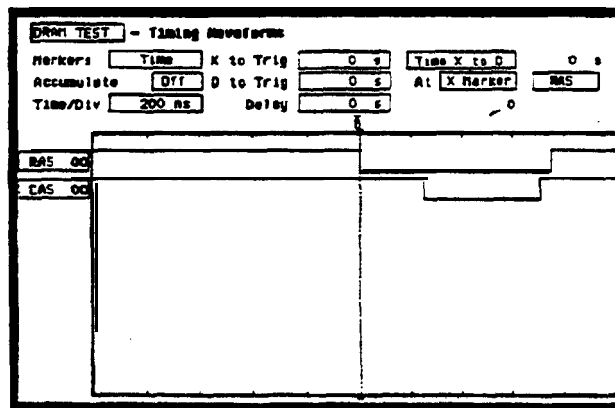


Figure 12-10. Changing Time/Div

Making the Measurement

What you want to know is how much time elapses between the time RAS goes low and the time CAS goes high again. You will use the X and 0 markers to quickly find the answer. Remember, you specified the negative-going edge of the RAS to be your trigger point; therefore, the X marker should be on this edge if X to Trig = 0. If not, follow steps 1 and 2.

1. Place the cursor on the X to Trig field and press SELECT . A pop-up will appear showing you the current time from the X marker to the trigger, however, you don't need to worry about this number now.
2. Rotate the KNOB to place the X marker on the negative-going edge of the RAS waveform and press SELECT . The pop-up closes and displays X to Trig = 0.000 s.
3. Place the cursor on 0 to Trig and press SELECT . Repeat step 2 except place the 0 marker on the positive-going edge of the CAS waveform and press SELECT. The pop-up closes and displays 0 to Trig = 710 ns.

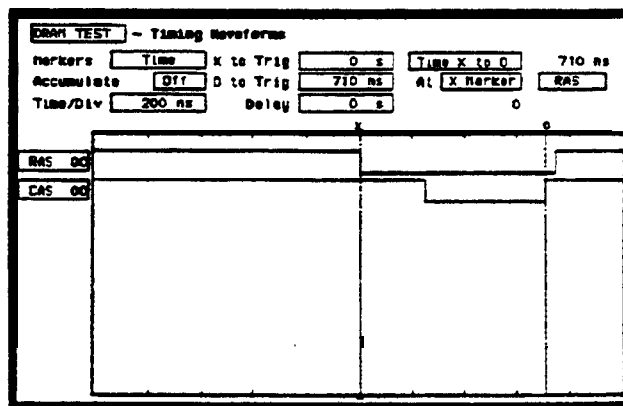


Figure 12-1 1. Marker Placement

Finding the Answer

Your answer could be calculated by adding the X to Trig and O to Trig times, but you don't need to bother. The logic analyzer has already calculated this answer and displays it in the Time X to O field.

This example indicates the time is 710 ns. Since the data book specifies a minimum of 250 ns, it appears your DRAM controller circuit is designed properly.

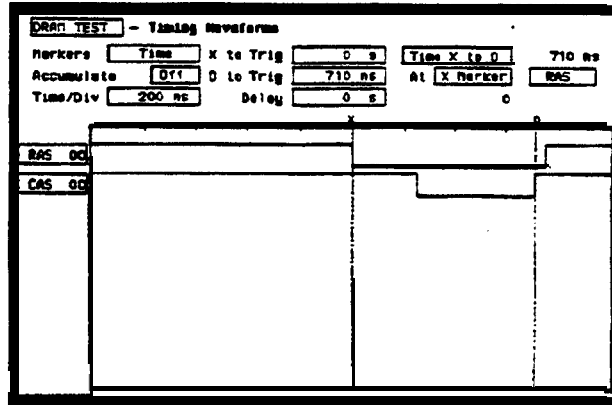


Figure 12-12. Time X to O

Summary

You have just learned how to make a simple timing measurement with the HP 1650A/51A logic analyzer. You have:

- specified a timing analyzer
- assigned pod 1
- assigned bits
- specified a trigger condition
- learned which probes to connect
- acquired the data
- configured the display
- set the Time/Div for best resolution
- positioned the markers for the measurement answer

You have seen how easy it is to use the timing analyzer to make timing measurements that you could have made with a scope. You can use the timing analyzer for any timing measurement that doesn't require voltage parametrics or doesn't go beyond the accuracy of the timing analyzer.

The State Analyzer

Introduction

This chapter introduces the state analyzer and contains the state analyzer menu maps.

- Chapter 14 explains the State Format menu
- Chapter 15 explains the State Trace menu
- Chapter 16 explains the State Listing menu
- Chapter 17 explains the State Compare menu
- Chapter 18 explains the State Chart menu
- Chapter 19 explains the State Waveform menu
- Chapter 20 gives you a basic State Analyzer Measurement example

The State Analyzer (An Overview)

The state analyzer acquires data synchronously using the system-under-test to clock the acquired data. The acquired data is displayed in a list form in the State Listing menu and in waveform form in the State Waveform menu. The state analyzer differs from the timing analyzer in that the acquisition clock is provided by the system-under-test instead of the internal acquisition clock used by the timing analyzer. Therefore, the State Waveform menu displays the state waveforms referenced by states per division and not seconds per division as in the timing analyzer.

State Analyzer Menu Maps

The State Analyzer menu maps show you the fields and the available options of each field within the six menus. The menu maps will help you get an overview of each menu as well as provide you with a quick reference of what each menu contains.

State Format Menu Map

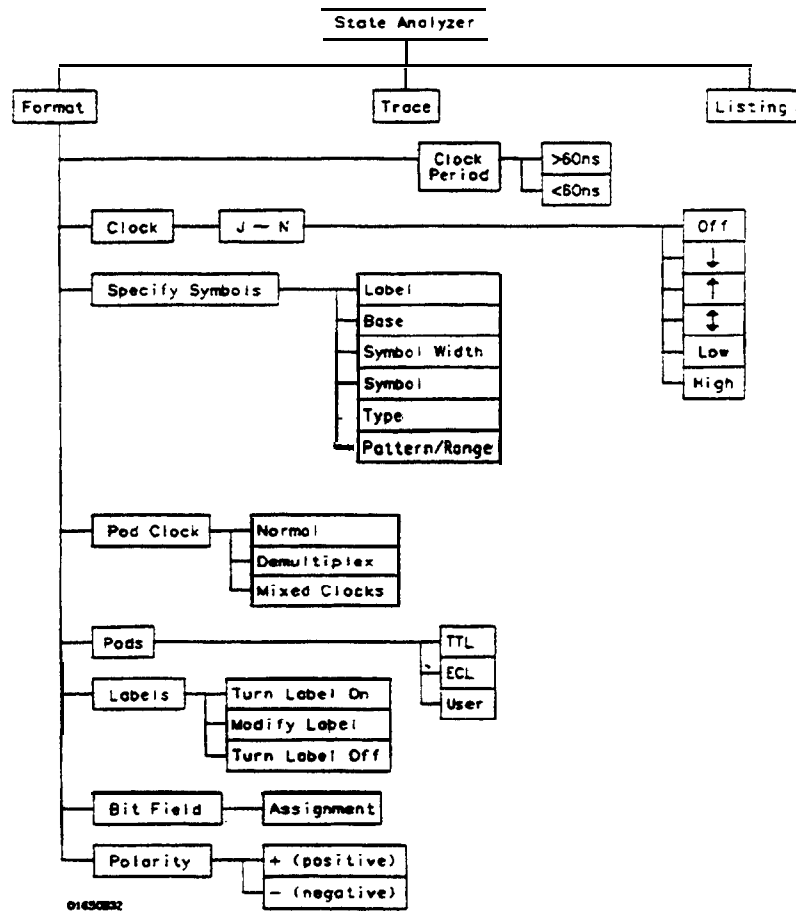


Figure 13-1. State Format Menu Map

State Trace Menu Map


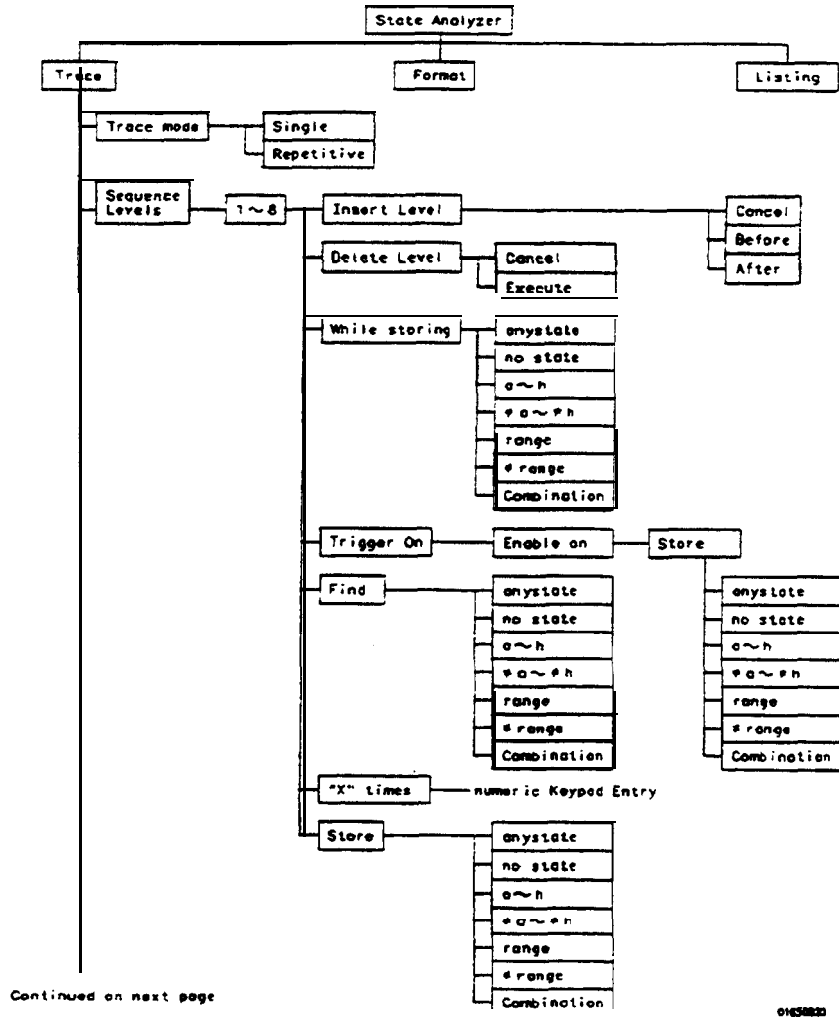


Figure 13-2. State Trace Menu Map

Continued from previous page

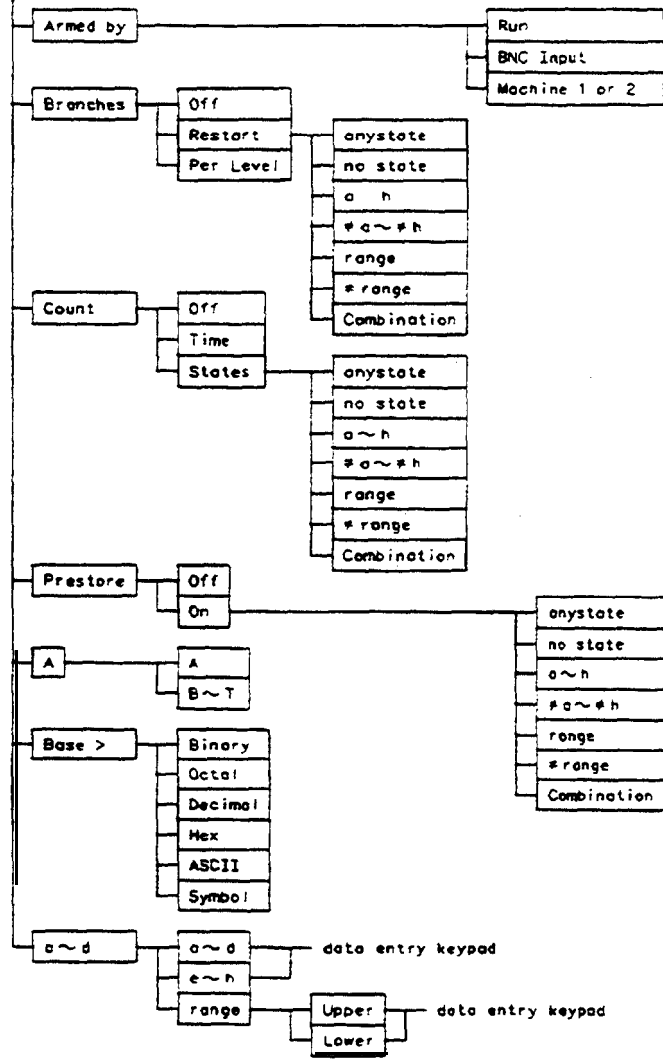

0160204

Figure 13-Z. State Trace Menu Map (continued)

State Listing Menu Map

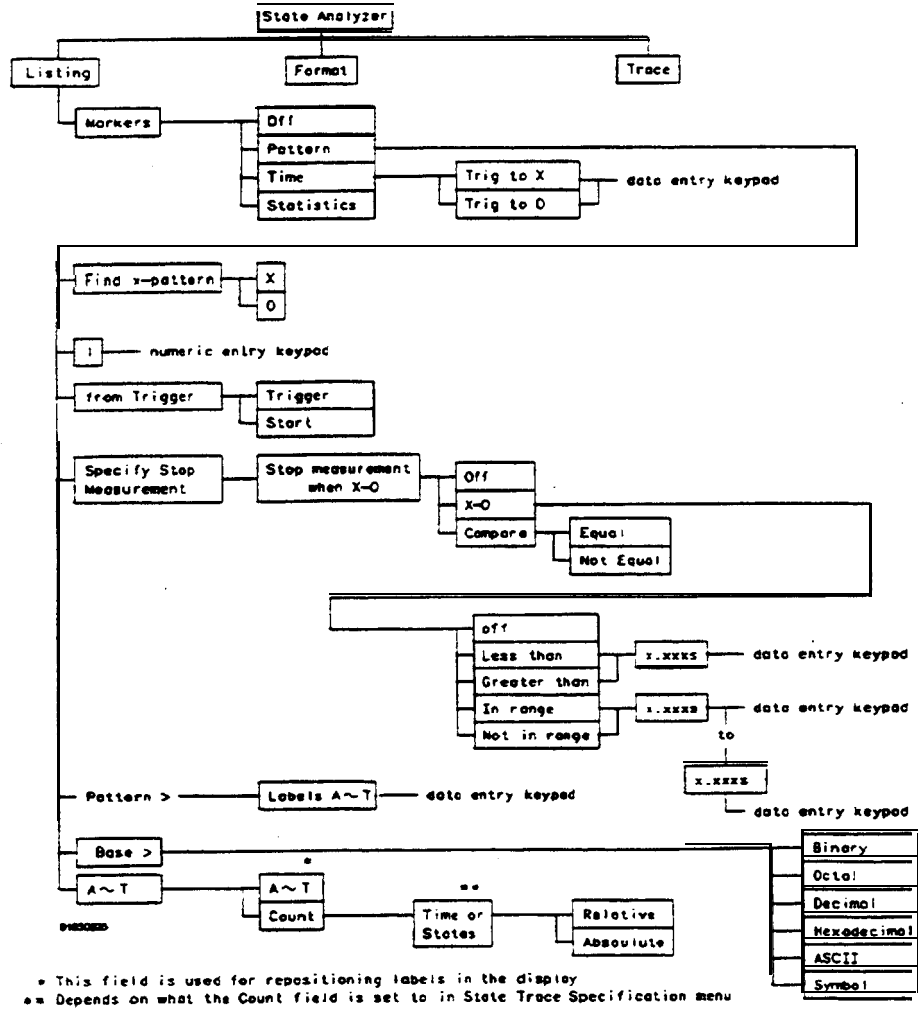


Figure 13-3. State Listing Menu Map

State Compare Menu Map

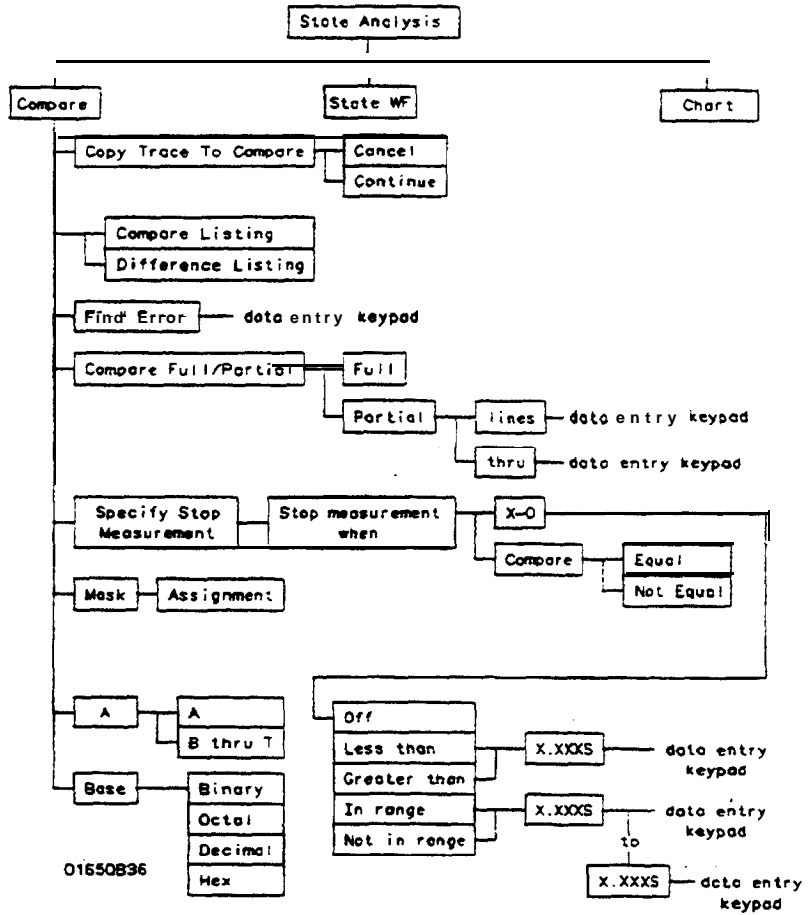


Figure 13-4. State Compare Menu Map

State Waveform Menu Map


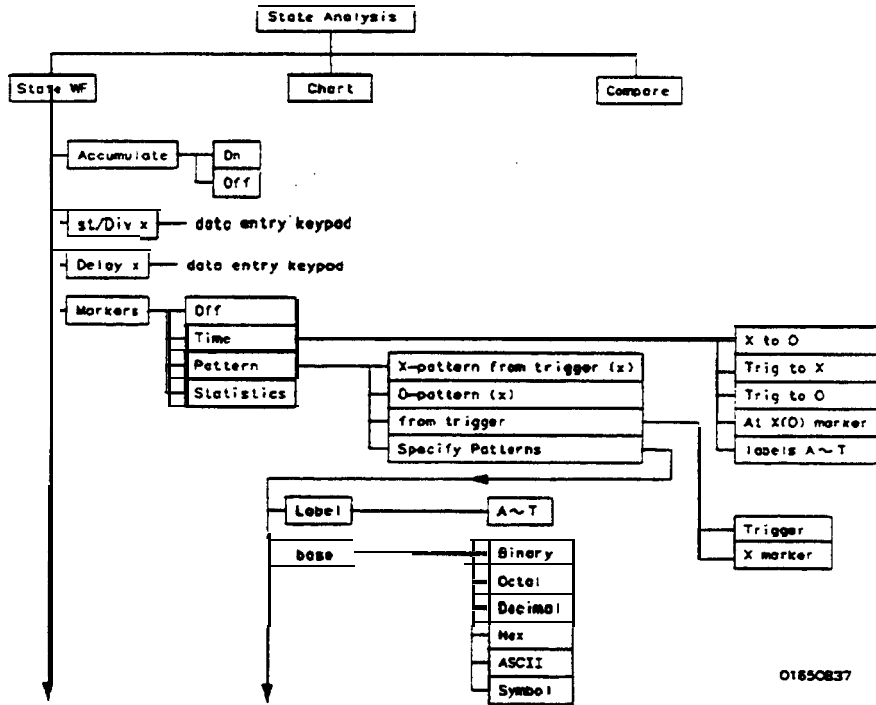



Figure 13-5. State Waveform Menu Map

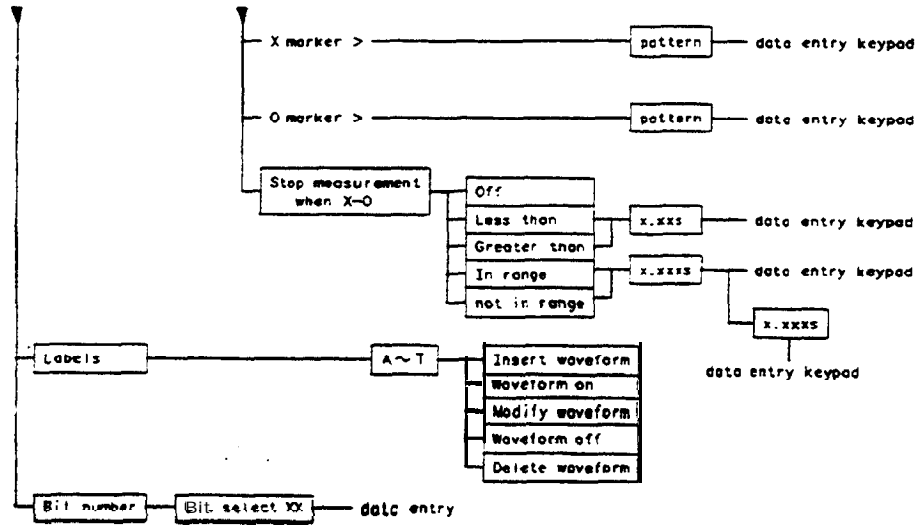

01650836

Figure 13-5. State Waveform Menu Map (continued)

State Chart Menu Map

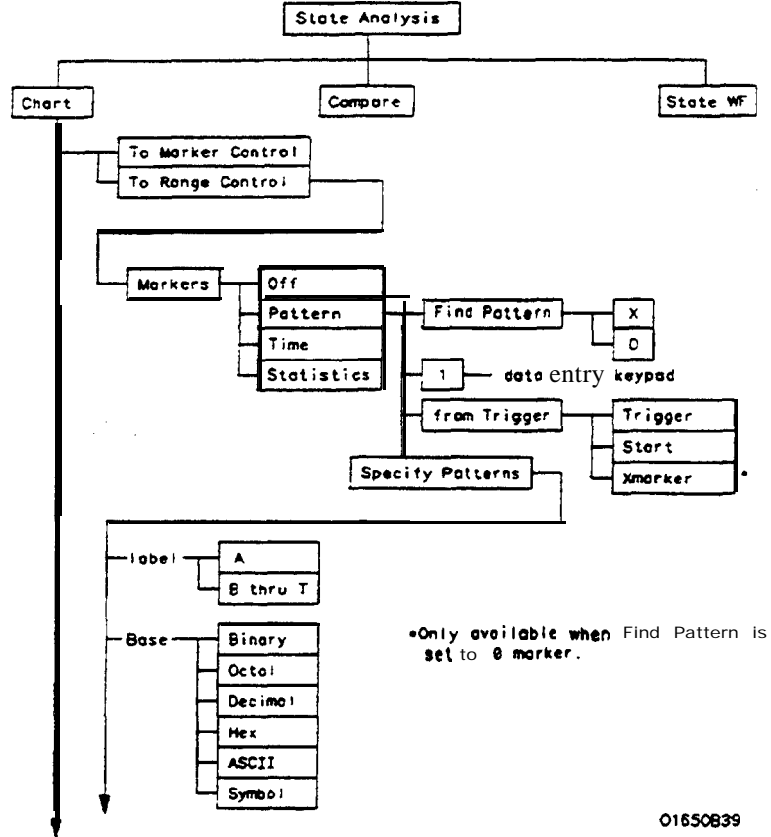

01650B39

Figure 13-6. State Chart Menu Map

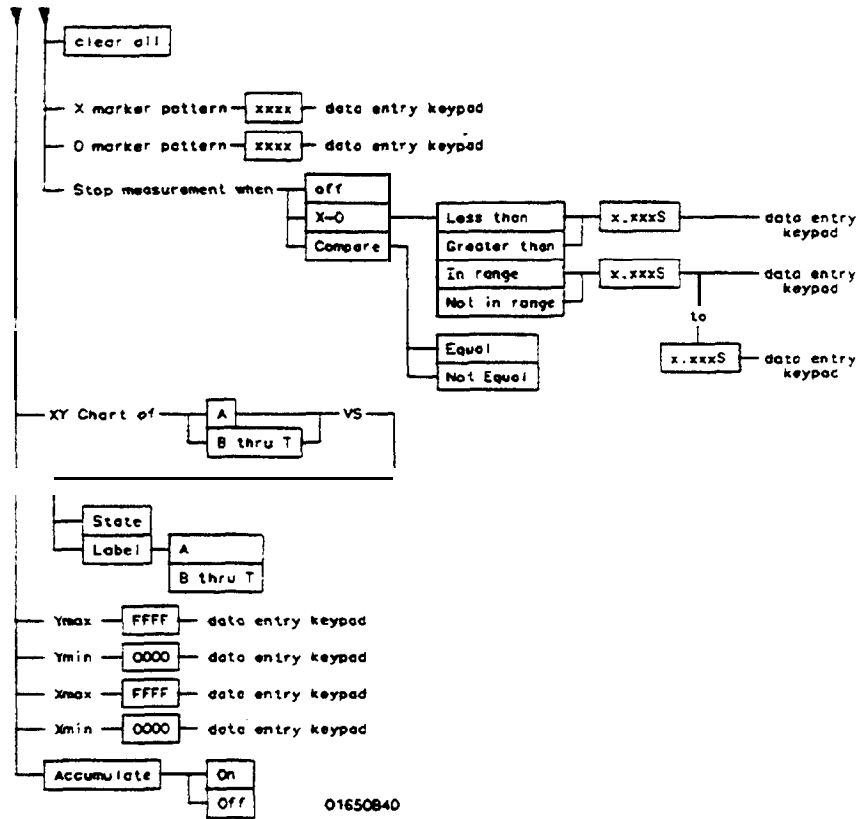


Figure 13-6. State Chart Menu Map (continued)

State Format Specification Menu

Introduction

This chapter **describes** the State Format Specification menu and **all pop-up menus that you will use on your state analyzer**. The purpose and functions of each menu are explained in detail, and we have included many illustrations **and examples** to make the explanations clearer.

Accessing the State Format Specification Menu

The State Format **Specification menu** can be accessed by **pressing the FORMAT key on the front panel**. If the **Timing Format Specification Menu** is displayed when you press the **FORMAT** key, you will have to **switch analyzers**. This is **not a problem**, it merely indicates that the last action you performed in the System Configuration Menu was on the **timing analyzer**.

State Format Specification Menu

The State **Format Specification** menu lets you **configure** the logic analyzer to **group channels from your microprocessor into labels you assign for your measurements**. You can set the threshold levels of the pods assigned to the state analyzer, assign labels and channels, specify symbols, and set clocks for triggering.

At power up, the logic analyzer is configured with a default setting. You can use this default setting to make a test measurement on the system under test. It can give you an idea of where to start your measurement. For an example of setting up configurations for the a State analyzer, refer to your *Getting Started* Guide or “State Analyzer Measurement Example” in Chapter 20 of this **manual**.

At power up the State Format Specification menu looks like that shown below

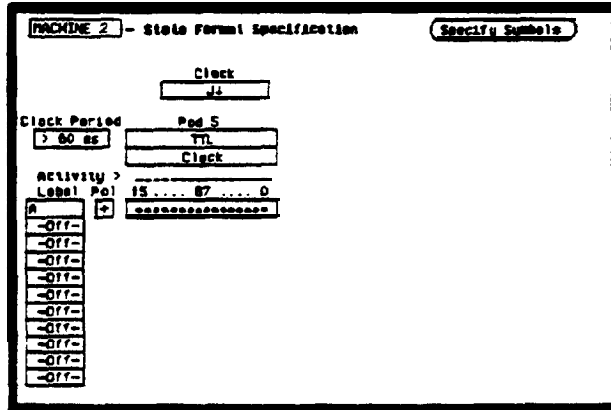




Figure 14-1. State **Format** Specification Menu

The State Format Specification menu for the HP 1651B is similar to that for the HP 1650B except that Pod 2 appears in the menu instead of Pod 5.

This menu shows only one pod assigned to each analyzer, which is the case at power up. Any number of pods can be assigned to one analyzer, from none to all five for the HP 1650B, and from none to two for the HP 1651B. In the State Format Specification menu, only three pods appear at a time in the display. To view any pods that are off screen, press the left/right ROLL key and rotate the KNOB. The pods are always positioned so that the lowest numbered pod is on the right and the highest numbered pod is on the left.

State Format Specification Menu Fields

Seven types of fields are present in the menus. They are:

-  Polarity (Pol)
- Bit assignments
- Pod threshold
- Specify Symbols
-  Podcbck
- Clock Period

A portion of the menu that is not a field is the Activity Indicators display. The indicators appear under the active bits of each pod, next to "Activity > ." When the logic analyzer is connected to your target system and the system is running, you will see ↓ in the Activity indicators display for each channel that has activity. These tell you that the signals on the channels are transitioning.

The fields in the Format menus are described in the following sections.

Label The label column contains 20 Label fields that you can define. Of the 20 labels, the state analyzer displays only 11 labels at one time. To view the labels that are off screen, press the up/down ROLL key and rotate the KNOB. The labels scroll up and down. To deactivate the scrolling, press the ROLL key again.

To access one of the Label fields, place the cursor on the field and press SELECT. You will see a pop-up menu like that shown below.




Figure 14-2. Label Pop-Up Menu

Turn Label On

Selecting this option turns the label on and gives it a default letter name. If you turned all the labels on they would be named A through T from top to bottom. When a label is turned on, bit assignment fields for the label appear to the right of the label under the pods.

Modify Label

If you want to change the name of a label, or want to turn a label on and give it a specific name, you would select the Modify label option. When you do, an Alpha Entry pop-up menu appears. You can use the pop-up menu and the keypad on the front panel to name the label. A label name can be a maximum of six characters.

Turn Label Off

Selecting this option turns the label off. When a label is turned off, the bit assignments are saved by the logic analyzer. This gives you the option of turning the label back on and still having the bit assignments if you need them. The waveforms and state listings are also saved.

You can give the same name to a label in the state analyzer as in the timing analyzer without causing an error. The logic analyzer distinguishes between them. An example of this appears in the *Getting Started Guide* and in chapter 20 of this manual.

Polarity (Pol) Each label has a polarity assigned to it. The default for all the labels is positive (+) polarity. You can change the polarity of a label by placing the cursor on the polarity field and pressing SELECT. This toggles the polarity between positive (+) and negative (-).

In the state analyzer, negative polarity inverts the data.

Bit Assignment The bit asst fields allow you to assign bits (channels) to labels. Above each column of bit assignment fields is a line that tells you the bit numbers from 0 to 15, with the left bit numbered 15 and the right bit numbered 0. This line helps you know exactly which bits you are assigning.

The convention for bit assignment is:

- (asterisk) indicates assigned
- (period) indicates unassigned

At power up the 16 bits of Pod 1 are assigned to the timing analyzer and the 16 bits of Pod 5 are assigned to the state analyzer.

To change a bit assignment configuration, place the cursor on a bit assignment field and press SELECT. You will see the following pop-up menu.




Figure 14-3. Bit Assignment Pop-Up Menu

Use the KNOB to move the cursor to an asterisk or a period and press SELECT. The bit assignment toggles to the opposite state of what it was before. When the bits (channels) are assigned as desired, place the cursor on Done and press SELECT. This closes the pop-up and displays the new bit assignment.

Assigning one channel per label may be handy in some applications. This is illustrated in chapter 8 of the *Getting Started Guide*. Also, you can assign a channel to more than one label, but this usually isn't desired.

Labels may have from 1 to 32 channels assigned to them. If you try to assign more than 32 channels to a label, the logic analyzer will beep, indicating an error, and a message will appear at the top of the screen telling you that 32 channels per label is the maximum.

Channels assigned to a label are numbered from right to left by the logic analyzer. The least significant assigned bit (LSB) on the far right is numbered 0, the next assigned bit is numbered 1, and so on. Since 32 channels can be assigned to one label at most, the highest number that can be given to a channel is 31.

Although labels can contain split fields, assigned channels are always numbered consecutively within a label. The numbering of channels is illustrated with the figure below.

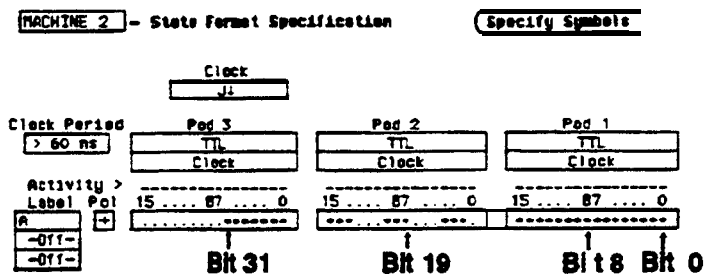


Figure 14-4. Numbering of Assigning Bits

Pod Threshold

Each pod has a threshold level assigned to it. For the HP 1651B Logic Analyzer, threshold levels may be defined for Pods 1 and 2 individually. For the HP 1650B Logic Analyzer, threshold levels may be defined for Pods 1, 2 and 3 individually, and one threshold for Pods 4 and 5. It does not matter if Pods 4 and 5 are assigned to different analyzers. Changing the threshold of one will change the threshold of the other.

If you place the cursor on one of the pod threshold fields and press SELECT, you will see the following pop-up menu.



Figure 14-s. Pod Threshold Pop-Up Menu

TTL sets the threshold at + 1.6 volts, and ECL sets the threshold at - 1.3 volts.

The User-defined option lets you set the threshold to a specific voltage between -9.9 V and $+9.9\text{ V}$. If you select this option you will see a Numeric Entry pop-up menu as shown.



Figure 14-6. User-defined Numeric Entry Pop-Up Menu

You can change the value in the pop-up either with the keypad on the front panel or with the KNOB, which you rotate until you get the desired voltage. When the correct voltage is displayed, press SELECT. The pop-up will close and your new threshold will be placed in the pod threshold field.

The threshold level you specify for the 16 data bits also applies to a pod's clock threshold.

Specify Symbols This field provides access to the Specify Symbols menu. It differs from the other fields in the State Format Specification menu in that it displays a complete menu instead of a pop-up. The complete description of the Specify Symbols Menu follows the State Format Specification Menu fields later in this chapter.

Clock The Clock field in the Format Specification menu displays the clocks for clocking your system. The display will be referred to as the "clocking arrangement."

The HP 1650B Logic Analyzer has five clock channels, each of which is on a pod. The clocks are connected through the pods simply for convenience. The clock channels are labeled J, K, L, M, and N and are on pods 1 through 5, respectively. The clocking of the state analyzer is synchronous with your system because your analyzer uses the signals present in your system. The signal you use must clock the analyzer when the data you want to acquire is valid.

The HP 1651B Logic Analyzer has two dock channels, each on one of the pods. The J clock is on pod 1 and the K clock is on pod 2.

When you select the Clock field, you will see the following pop-up menu with which you specify the clock.

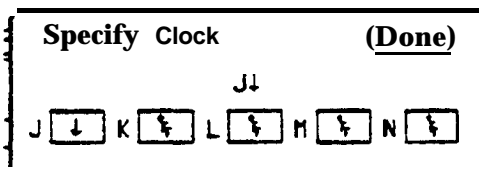


Figure 14-7. Clock Pop-Up Menu

You can use one of the clocks alone or combine them to build one clocking arrangement. If you select a field to the right of one of the clocks in the pop-up you will see another pop-up menu:

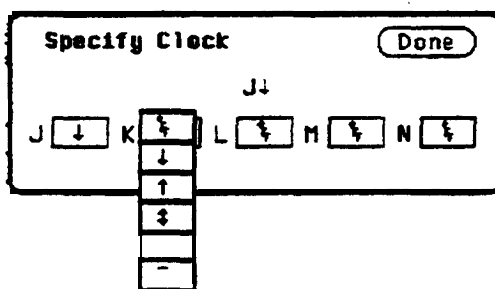


Figure 14-8. Single Clock Pop-Up Menu

You can specify the negative edge of the clock, the positive edge either edge, a high level, a low level, or the clock to be off.

The clocks are combined by ORing and ANDing them. Clock edges are ORed to clock edges, clock levels are ORed to clock levels, and clock edges are ANDed to clock levels.

For example, if you select ↓ for the J clock, ↑ for the K clock, _ for the M clock, and - for the N clock, the resulting clocking arrangement will appear in the display as:

$$\text{Clock} \\ \boxed{(J\downarrow + K\uparrow) \cdot (M_ + N^-)}$$

Figure 14-9. Example of a Clocking Arrangement

With this arrangement, the state analyzer will clock the data when there is a negative edge of the J clock OR a positive edge of the K clock, AND when there is a low level on the M clock OR a high level on the N clock.

You must always specify at least one clock edge. If you try to use only clock levels, the logic analyzer will display a message telling you that at least one edge is required.

Pod Clock

Your logic analyzer has the capability of docking data in three different ways. The pod Clock Fields in the State Format Specification menu allow you to specify which of the three ways you want to clock the data.

Each pod assigned to the state analyzer has a pod Clock field associated with it. Selecting one of the pod Clock fields gives you the following pop-up menu:




Figure 14-10. Pod clock Field Pop-Up Menu

Normal

This option specifies that clocking will be done in single phase. That is the clocking arrangement located in the Clock field above the pods in the State Format Specification menu will be used to clock all the pods assigned to this machine.

For example, suppose that the Clock field looks like the following:




Figure 14-11. Example of a Clocking Arrangement

In Normal mode the state analyzer will sample the data on any assigned pods on a negative edge of the J clock OR on a positive edge of the K clock.

Demultiplex

With the HP 1650B/51B Logic Analyzers, you can clock two different types of data that occur on the same lines. For instance, lines that transfer both address and data information need to be clocked at different times in order to get the right information at the right time. The Demultiplex option provides the means to do this.

When you select the Demultiplex option, the pod Clock field changes to "Master | Slave," and two clock fields appear above the pods where just one Clock field used to be. These fields are the Master Clock and Slave Clock, as shown:

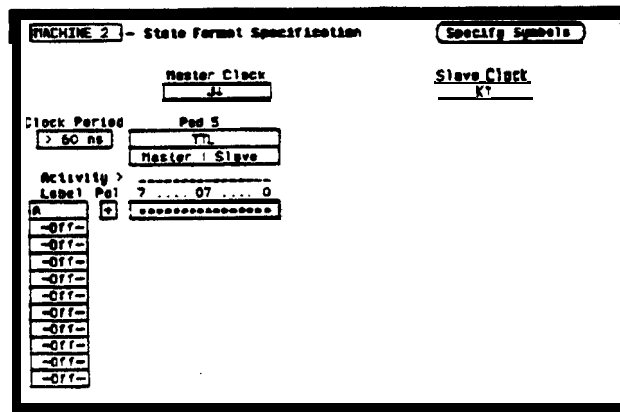


Figure 14-12. Master Clock and Slave Clock

Demultiplexing is done on the data lines of the specified pod to read only the lower eight bits. This is two-phase clocking, with the Master Clock following the Slave Clock. The analyzer first looks for the clocking arrangement that you specify in the Slave Clock. When it sees this arrangement, the analyzer clocks the data present on bits 0-7 of the pod, then waits for the clocking arrangement that you specify in the Master Clock. When it sees this arrangement, it again clocks the data present on bits 0-7 of the pod. The upper eight bits of the pods are ignored and don't need to be connected to your system.

Notice, the bit numbers that appear above the bit assignment field have changed. The bits are now numbered 7...07...0 instead of 15...87...0. This helps you set up the analyzer to clock the right information at the right time.

The address/data lines AD0-AD7 on the 8085 microprocessor are an example of Demultiplex. During part of the operating time the lines have an address on them, and during other times they have data on them. Hook the lower eight bits of one of the pods to these eight lines and set the Slave and Master Clocks so that they clock the data and the address at the proper time.

In this example, you may choose to assign the bits in the State Format Specification menu similarly to that shown below. In this case you would want to clock the address with the Slave Clock and the data with the Master Clock.

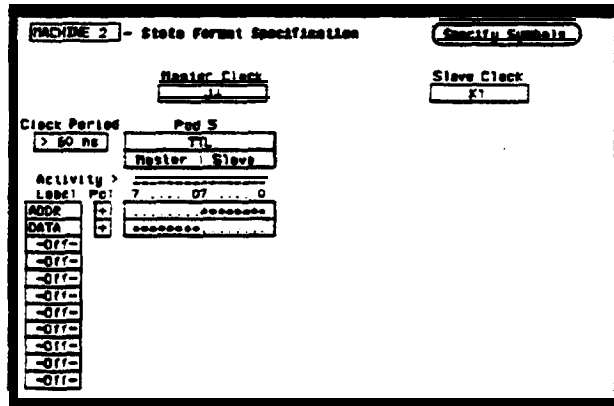


Figure 14-13. Master and Slave Clock Bit Assignments

The Master and Slave Clocks can have the same clocking arrangements. The clocking is still done the same way, with the lower eight bits being clocked first on the Slave Clock, then on the Master Clock.

Mixed Clocks

The Mixed Clocks option allows you to dock the lower eight bits of a pod separately from the upper eight bits. The state analyzer uses Master and Slave Clocks to do this. If you select this option from the pod Clock pop-up, the pod Clock field changes to Master | Slave," and two Clock fields, Master and Slave, appear above the pods.

As in **Demultiplex**, the Master Clock follows the Slave Clock. The state analyzer looks for the clocking arrangement given by the Slave Clock and clocks the lower eight bits. Then it looks for the clock arrangement given by the Master Clock and clocks the upper eight bits. Unlike **Demultiplex**, all 16 bits of a pod are sampled.

The Master and Slave Clocks can have the same clocking arrangements. The clocking is still done the same way, with the lower eight bits clocked on the Slave Clock and the upper eight bits clocked on the Master Clock.

Clock Period

This field provides greater measurement accuracy when your state input clock period is greater than 60 ns. When you select > 60 ns, the state analyzer provides greater immunity against noise or ringing in the state input clock signal; also, the logic analyzer provides greater accuracy when triggering another state or timing analyzer or the BNC trigger out.

If your State input clock period is less than 60 ns, you should select < 60 ns. This and disables the Count field in the State Trace Specification menu because the maximum clock rate when counting is 16.67 MHz (60 ns clock period). This also turns Prestore off.

Specify Symbols Menu

The logic analyzer supplies Timing and State Symbol Tables in which you can define a mnemonic for a specific bit pattern of a label. When measurements are made by the state analyzer, the mnemonic is displayed where the bit pattern occurs if the Symbol base is selected.

It is possible for you to specify up to 200 symbols in the logic analyzer. If you have only one of the internal analyzers on, all 200 symbols can be defined in it. If both analyzers are on, the 200 symbols are split between the two. For example, analyzer 1 may have 150, leaving 50 available for analyzer 2.

To access the Symbol Table in the State Format Specification menu, place the cursor on the Specify Symbols field and press SELECT. You will see a new menu as shown. This is the default setting for the Symbol Table in both the timing and state analyzers.

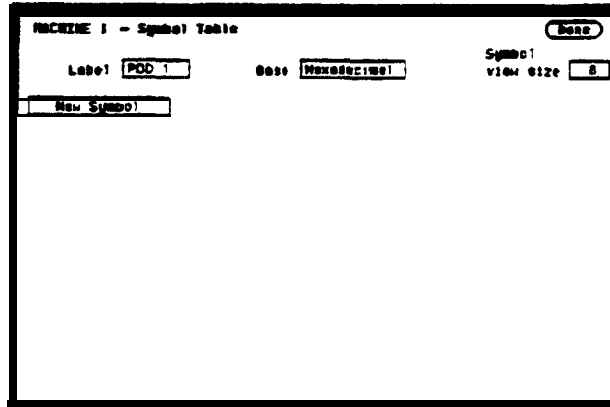


Figure 14-14. Symbol Table Menu

Specify Symbols Menu Fields

There are four fields in the Symbol Table menu. They are:

- Label
- Base
- Symbol view size
- Symbol name

Label The Label field identifies the label for which you are specifying symbols. If you select this field, you will get a pop-up that lists all the labels turned on for that analyzer.




Figure 14-15. Label Pop-Up Menu

Each label has a separate symbol table. This allows you to give the same name to symbols defined under different labels. In the Label pop-up select the label for which you wish to specify symbols.

Base The Base field tells you the numeric base in which the pattern will be specified. The base you choose here will affect the pattern field of the State Trace Specification menu. This is covered later in this chapter.

To change the base, place the cursor on the field and press SELECT. You will see the following pop-up menu.




Figure 14-16. Base Pop-Up Menu

If more than 20 channels are assigned to a label, the Binary option is not offered in the pop-up. The reason for this is that when a symbol is specified as a range, there is only enough room for 20 bits to be displayed on the screen.

Decide which base you want to work in and choose that option from the numeric Base pop-up menu.

If you choose the ASCII option, you can see what ASCII characters the patterns and ranges defined by your symbols represent. ASCII characters represented by the decimal numbers 0 to 127 (hex 00 to 7F) are offered on your logic analyzer. Specifying patterns and ranges for symbols is discussed in the next section.



You cannot specify a pattern or range when the base is ASCII. First define the pattern or range in one of the other bases, then switch to ASCII to see the ASCII characters.

Symbol View Size The Symbol view size field lets you specify how many characters of the symbol name will be displayed when the symbol is referenced in the State Trace Specification menu and the State Listing menu. Selecting this field gives you the following pop-up.




Figure 14-17. Symbol View Sii Pop-Up Menu

You can have the logic analyzer display from 3 to all 16 of the characters in the symbol name. For more information see "State Trace Specification Menu" and "State listing Menu" later in this chapter.

Symbol Name When YOU first access the Symbol Table, there are no symbols specified. The symbol name field reads "New Symbol." If you select this field, you will see an Alpha Entry pop-up menu on the display. Use the pop-up menu and the keypad on the front panel to enter the name of your symbol. A maximum of 16 characters can be used in a symbol name.

When you select the Done field in the Alpha Entry pop-up menu the name that appears in the symbol name field is assigned and two more fields appear in the display.




Figure 14-18. Symbol Defined as a Pattern

The first of these fields defines the symbol as either a Pattern or a Range. If you place the cursor on this field and press SELECT, it will toggle between Pattern and Range.

When the symbol is defined as a pattern, one field appears to specify what the pattern is. Selecting this field gives you a pop-up with which you can specify the pattern. Use the keypad and the DONT CARE key on the front panel to enter the pattern. Be sure to enter the pattern in the numeric base that you specified in the Base field.



Figure 14-19. Specify Pattern Pop-Up Menu

If the symbol is defined as a range, two fields appear in which you specify the upper and lower boundaries of the range.

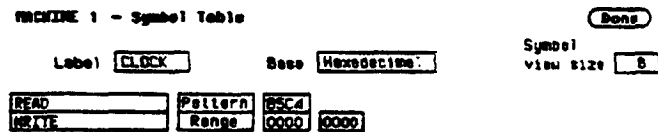


Figure 14-20. Symbol Defined as a Range

Selecting either of these fields gives you a pop-up with which you can specify the boundary of the range.




Figure 14-21. Specify Range Pop-Up Menu

You can specify ranges that overlap or are nested within each other. Don't cares are not allowed.

To add more symbols to your symbol table, place the cursor on the last symbol defined and press SELECT. A pop-up menu appears as shown.




Figure 14-22. Symbol Pop-Up Menu

The first option in the pop-up is Modify symbol. If you select this option, you will see an Alpha Entry pop-up menu with which you can change the name of the symbol.

The second option in the pop-up is Insert new symbol. It allows you to specify another symbol. When you select it, you will see an Alpha Entry pop-up menu. Use the menu and the keypad on the front panel to enter the name of your new symbol. When you select Done, your new symbol will appear in the Symbol Table. The third option in the pop-up is Delete symbol. If you select this option, the symbol will be deleted from the Symbol Table.

Leaving the Symbol Table Menu

When you have specified all your symbols, you can leave the Symbol Table menu in one of two ways. One method is to place the cursor on the Done field and press SELECT. This puts you back in the Format Specification menu that you were in before entering the Symbol Table. The other method is to press the FORMAT, TRACE, or DISPLAY keys on the front panel to get you into the respective menu.

State Trace Menu

Introduction

This chapter describes the State Trace menu and the pop-up menus that you will use on your state analyzer. The purpose and functions are described in detail, and we have included many illustrations and examples to make the explanations clearer.

The Trace Specification menu allows you to configure the state analyzer to capture only the data of interest for your measurement. In the state analyzer you can configure the analyzer to trigger on a sequence of states. The default setting is shown in figure 15-1 below.

For an example of setting up a trace configuration for a State analyzer, refer to your *Getting Started Guide* or State Analyzer Measurement Example" in Chapter 20 of this manual.

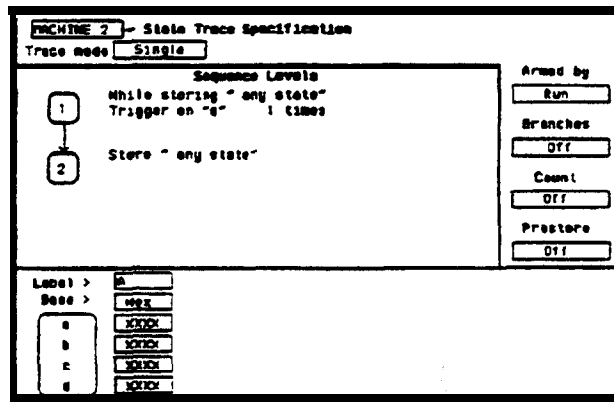


Figure 15-1. State Trace Specification Menu

Accessing the State Trace Menu

The State Trace menu can be accessed by pressing the TRACE key on the front panel. If the Timing Trace Specification menu is displayed when you press the TRACE key, you will have to switch analyzers. This is not a problem, it merely indicates that the last action you performed in the System Configuration Menus was on the timing analyzer.

State Trace Menu Fields

The menu is divided into three sections: the Sequence Levels in the large center box, the acquisition fields at the top and right of the screen, and the qualifier and pattern fields at the bottom of the screen.

Before describing the fields in the menu, we need to define a few terms. These terms will be used in the discussions of the fields, so understanding their meanings is essential.

Pattern Recognizers: a pattern of bits (0, 1, or X) in each label. There are eight recognizers available when one state analyzer is on. Four are available to each analyzer when two state analyzers are on. The pattern recognizers are given the names a through h and are partitioned into groups of four, a-d and e-h.

Range Recognizer: recognizes data which is numerically between or on two specified patterns. One range term is available and is assigned to the first state analyzer created by assigning pods to it or if only one analyzer is on, then the range term is assigned to it.

Qualifier: user-specified term that can be anystate, nostate, a single pattern recognizer, a range recognizer, the complement of a pattern or range recognizer, or a logical combination of pattern and range recognizers. When you select a field to specify a qualifier, you will see the following qualifier pop-up menu.

any state
no state
a
b
c
d
e
f
g
h
ab
ac
ad
ae
af
ag
ah
range
all range
Combinations

Figure 15-2. Qualifier Pop-Up Menu

If you select the Combination option in the pop-up, you will see a pop-up similar to that shown below.

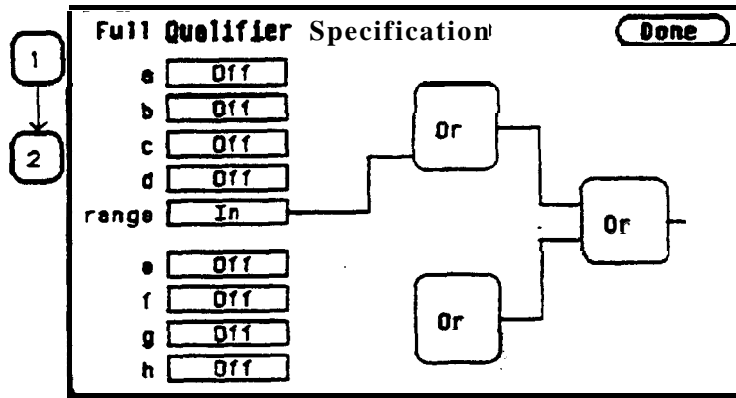



Figure 15-3. Full Qualifier Specification Pop-Up

Note 

If two multi-pod state analyzers are on, the qualifier pop-up menu will show that only four pattern recognizers are available to each analyzer. Pattern recognizers a-d and the range recognizer are assigned to the first analyzer created, and pattern recognizers e-h go with the second analyzer. In the Full Qualifier Specification pop-up there will be only one OR gate and one set of pattern recognizers.

With this Full Qualifier Specification pop-up, you specify a logical combination of patterns or ranges as the qualifier. The pattern recognizers are always partitioned into the groups of four shown. Only one operator is allowed between the patterns in a group. Patterns in uncomplimented form (a, b, etc.) can only be ORed.

The complements of patterns (\neq a, \neq b, etc.) can only be ANDed. For example, if the first OR field (gate) is changed to AND, all the patterns for that gate are complemented, as shown below.

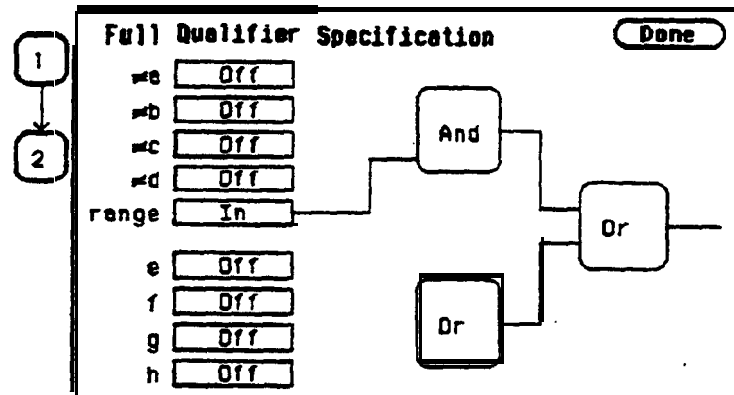


Figure 15-4. Complemented Patterns

To specify a pattern to be used in the combination, place the cursor on the pattern recognizer field and press SELECT. The field toggles from Off to On and a connection is drawn from the pattern field to the gate. In figure 15-5, patterns b, c and d and the range are ORed together, and e and g are ANDed together.

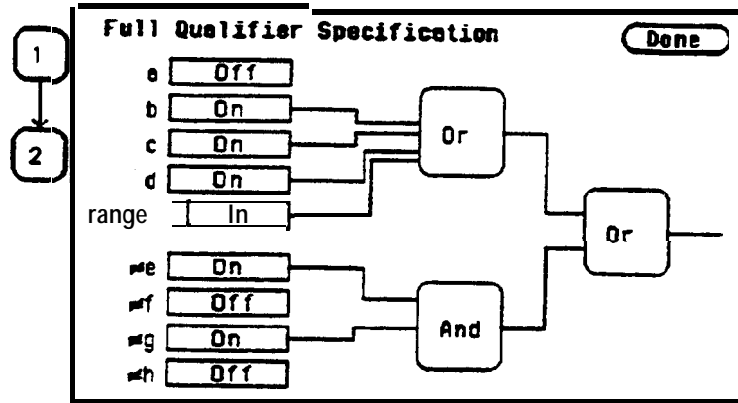


Figure 15-5. Patterns Assigned for Logical Combinations

As shown in the previous figures, the range is included with the first group of patterns (a-d). If you select the range field, you will see the following pop-up menu.

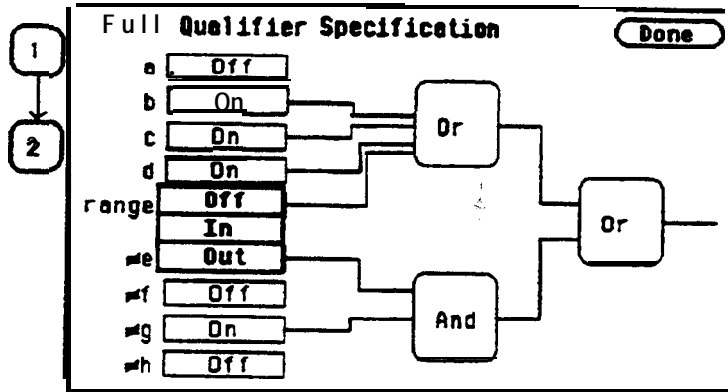


Figure 15-6. Range Specification Pop-Up Menu

Off disconnects the range from the qualifier specification. In indicates that the contents of the range are to be in the qualifier specification, and Out indicates that the complement of the range is to be in the qualifier specification.

When you have specified your combination qualifier, select Done. The Fall Qualifier Specification pop-up closes and the Boolean expression for your qualifier appears in the field for which you specified it.

While storing (b+c+d+range)+(e+f+g)


Figure 15-7. Boolean Expression for Qualifier

Sequence Levels

There are eight trigger sequence levels available in the state analyzer. You can add and delete levels so that you have from two to eight levels at a time.

Only three levels appear in the Sequence Levels display at one time. To display other levels so that they can be accessed, press the up/down ROLL key and rotate the KNOB.

If you select level 1 shown in figure 15-1, you will see the following pop-up menu:

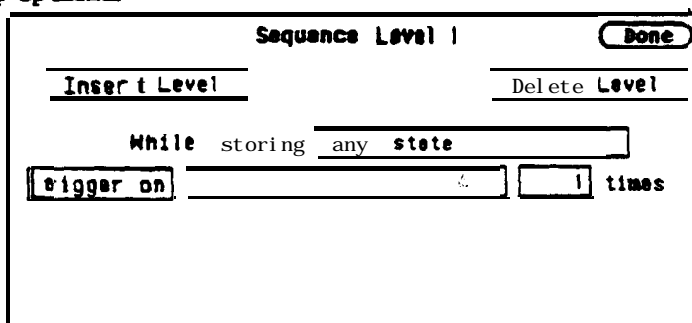

The image shows a pop-up menu titled "Sequence Level 1" with a "Done" button in the top right corner. Below the title, there are two buttons: "Insert Level" on the left and "Delete Level" on the right. In the center, there is a text field containing "While storing any state". Below this, there is a button labeled "Trigger on" followed by a text field containing "1" and the word "times".

Figure 15-8. Sequence Level Pop-up Menu

Not all sequence level pop-up menus look like this one. This happens to be the trigger sequence level in which you specify the state on which the analyzer is to trigger. The trigger term can occur in any of the first seven levels, and it is not necessarily a selectable field. The fields in the menu of figure 15-8 are described on the following pages.

Insert level To insert a level, place the cursor on the field labeled **Insert Level** and press **SELECT**. You will see the following pop-up menu.




Figure 15-0. Insert Level Pop-Up Menu

Cancel returns you to the sequence level pop-up without inserting a level. **Before** inserts a level before the present level. **After** inserts a level after the present level. If there are eight levels, the **Insert Level** field doesn't appear in the sequence level pop-ups.

Delete Level If you want to delete the present level, select the field labeled **Delete Level**. You will see a pop-up menu with the choices **Cancel** and **Execute**. **Cancel** returns you to the sequence level pop-up without deleting the level. **Execute** deletes the present level and returns you to the **State Trace Specification** menu.

Note 

If there are only two levels, neither field can be deleted even though the **Delete Level** field still appears in the menu. There will always be a trigger term level and a store term level in **Sequence Levels**. Therefore, if you try to delete either of these, all terms you have specified in these levels will be set to default terms, and, the trigger and store term levels will remain.

Storage Qualifier Each sequence level has a storage qualifier. The storage qualifier specifies the states that are to be stored and displayed in the State Listing. Selecting this field gives you the qualifier pop-up menu shown in figure 15-2, with which you specify the qualifier.

As an example, suppose you specify the storage qualifier in a sequence level as shown below.

While storing

Figure 15-10. Storage Qualifier Example

The only states that will be stored and displayed are the states given by pattern recognizers a and d.

Branching Qualifier Every sequence level except the last has a primary branching qualifier. With the branching qualifier, you tell the analyzer to look for a specific state or states. The primary branching qualifier advances the sequencer to the next level if its qualifier is satisfied.

In the example of figure 15-8, the branching qualifier tells the analyzer when to trigger. In other sequence levels, the qualifier may simply specify a state that the analyzer is to look for before continuing to the next level.

Some sequence levels also have a secondary branching qualifier. The secondary branch will, if satisfied, route the sequencer to a level that you define. This is covered in more detail in "Branches" later in this chapter.

Occurrence Counter

The primary branching qualifier has an occurrence counter. With the occurrence counter field you specify the number of times the branching qualifier is to occur before moving to the next level.

To change the value of the occurrence counter, position the cursor on the field and either press SELECT or press a numeric key on the front-panel keypad. You will see a pop-up similar to that shown below.

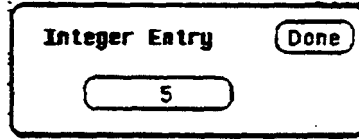


Figure 15-11. Occurrence counter Pop-Up Menu

You can change the value by either rotating the KNOB or pressing the appropriate numeric keys. The qualifier can be specified to occur from one to 65535 times.

Storage Macro

Your logic analyzer has the capability of post-trigger storage through a storage macro. The storage macro is available only in the second to last level, and it consumes both that level and the last level. The field in figure 15-8 allows you to configure the state analyzer for post-trigger storage. This field does not always say Trigger on. If the sequence level is not a trigger level, the field will say Then find, as shown below.



Figure 15-12. Then Find Branching Qualifier

Selecting the field gives you a pop-up with two options. One option is what the field said previously. The other option is **Enable on**. If you select this option, the Sequence Level pop-up changes to look similar to that shown below.

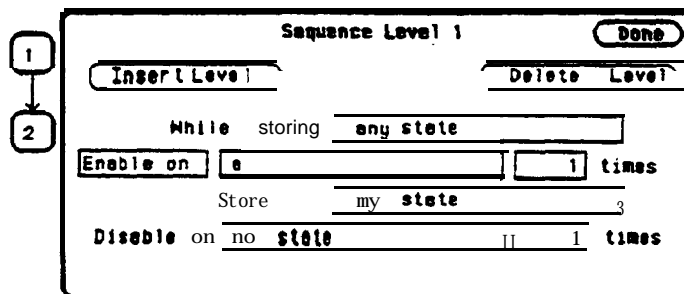


Figure 15-13. Storage Macro Sequence Level Example

Note 

Enable on can only be the next to last term, and when on, the last term is combined with the **Enable** term.

You specify qualifiers for the states on which you want the macro to enable, the states you want to store, and the states on which you want the macro to disable. The storage macro is a loop that keeps repeating itself until memory is full. The loop is repeated when the disable qualifier is satisfied. As an example, suppose you configure the sequence level of figure 15-13 to look like that shown below.

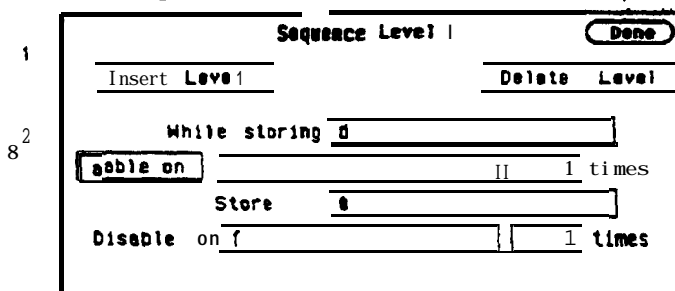


Figure 15-14. Sequence Level Pop-up with Storage Macro

The logic analyzer will store the state given by pattern recognizer d until it comes across the state given by a. When it sees state a, the logic analyzer starts to store the state given by pattern recognizer e. It stores that state until it sees the state given by f, at which time it disables and starts the process all over again. The analyzer repeats this process until its memory is full.

Reading the Sequence Level Display

Reading the display is fairly straightforward. For example, suppose your display looks like that shown below.

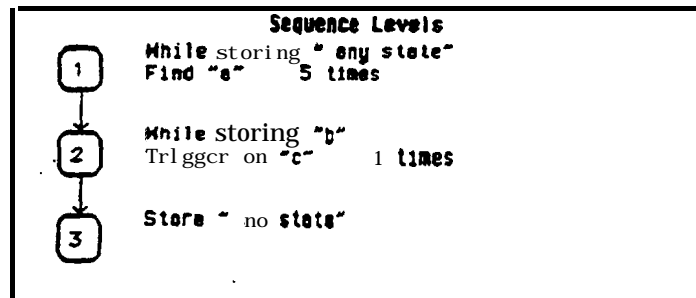


Figure 15-15. Sequence Level Display Example

In level 1 any state is stored while the logic analyzer searches for five occurrences of the pattern given by pattern recognizer a. When the five occurrences are found, the sequencer moves on to level 2. In level 2 the state given by pattern recognizer b is stored until one occurrence of the pattern given by pattern recognizer c is found and the logic analyzer triggers. In level 3 no state is stored, so the last state stored is the trigger state.

An example of a state listing for the previous State Trace configuration is shown below. The state patterns specified are:

- a = B03C
- b = 0000
- c = 8930

MACHINE 2 - STATE LISTING

Label	>	A
Base	>	Hex
-0028		4E75
-0027		61B6
-0026		W 0 0
-0025		88C9
4 0 2 4		B03C
-0023		00FF
4 0 2 2		M 0
4 0 2 1		0 0
4 0 2 0		4E75
-0019		3000
-0018		+□□
4 0 1 7		W 0 0
-0016		B03C
-0015		00FF
-0014		67F8
4 0 1 3		B03C
-0012		61FA
-0011		B03C
-0010		□□□□
-0009		8930
-0008		4E7A
-0007		7F9A
-0006		61B6
-0005		B03C
4 0 0 4		0000
4 0 0 3		0000
-0002		□□□□
-0001		□□□□
+0000		8930

Figure 1646. State Listing Example

Anystate was stored while the analyzer looked for five occurrences of the state B03C. After the fifth occurrence was found, only state 0000 was stored until state 8930 was found, and the analyzer triggered. After the trigger, no states were stored.

Acquisition Fields

The acquisition fields are comprised of the Trace mode, Armed by, Branches, Count, and Restore fields, as shown below.

MACHINE 2 - State Trace Specification

Trace mode

Sequence Levels

1 While storing - any state
Trigger on "0" 1 times

2 Store - any state

Armed by

Branches

Count

Restore

Figure 15-17. State Trace Acquisition Fields

Trace Mode You specify the mode in which the state analyzer will trace with the Trace mode field. You have two choices for trace mode: Single and Repetitive. If you place the cursor on the field and press SELECT the field toggles from one mode to the other.

Single Trace mode acquires data once per trace. Repetitive Trace mode repeats single acquisitions until the STOP key on the front panel is pressed, or if Stop measurement is on, until conditions specified with the X and O markers in the State Listing menu are met.

If both analyzers are on, only one trace mode can be specified. Specifying one trace mode for one analyzer sets the same trace mode for the other analyzer.

Armed By The Armed by field lets you specify how your state analyzer is to be armed. The analyzer can be armed by the RUN key, the other analyzer, or an external instrument through the BNC Input port. Any of these can tell the analyzer when to start capturing data.

When you select the Armed by field, a pop-up menu appears like that shown below. The first two options always appear in the pop-up. The third option will give the name of the other analyzer. If the other analyzer is off, or if the other machine is being armed by this machine, this option will not be available.




Figure 15-18. Armed By Pop-Up Menu

Branches

The Branches field allows you to configure the sequencer of the state analyzer to branch from one sequence level to another with secondary branching qualifiers, or to restart when a certain condition is met. Selecting this field gives you the following pop-up menu.




Figure S-19. Branches Pop-Up Menu

Off

If you select Off, all secondary branching qualifiers are deleted from the sequence levels. Only the primary branches remain.

Restart

The Restart option allows you to start over from sequence level 1 when a specified condition is met. This can be handy if you have code that branches off in several paths and you want the analyzer to follow one certain path. If the analyzer goes off on an undesired path, you would want the analyzer to stop and go back to the beginning and take the correct path.

If you select the Restart option, you will see a qualifier pop-up menu like that shown in figure 15-2. With the pop-up you select the qualifier for the pattern on which you want your analyzer to start over.

When your state analyzer is reading data it proceeds through the sequence. If a term doesn't match the branching qualifier, it is then checked against Restart. If the term matches, the state analyzer jumps back the sequence level 1.

Per Level

Selecting the Per level option allows you to define a secondary branching qualifier for each sequence level. A statement is added in each level so that you can configure the analyzer to move to a different level when a specified condition is met. An example of a sequence level with a secondary branching qualifier is shown in the figure below.

Sequence Level 2		(Done)
<u>Insert Level 1</u>	<u>Delete Level</u>	
While storing <u>b</u>		
Then find	<u>c</u> <u>1</u> times	
Else on	<u>f</u> got0 level	<u>4</u>

Figure 15-20. Secondary Branching. Qualifier

With this configuration, the state analyzer will store b until it finds c. If it finds f before it finds c, it will branch to sequence level 4. If you have specified a storage macro in the next to last sequence level the Else on statement will not appear in that level since a secondary branching qualifier already exists for that level.

In the last sequence level, which only specifies states that are to be stored, the secondary branching qualifier statement looks like that shown below.

Sequence Level 7		(Done)
Insert Level		Delete Level
store	any state	
On	a	got0 level 6

Figure 15-21. Secondary Branch Qualifier in Last Level

In this example, as the state analyzer stores anystate, it will branch to sequence level 6 if it finds the state given by qualifier e.

The trigger sequence level is used as a boundary for branching between levels. This level and the levels that occur before it cannot branch to levels that occur after the trigger level, and vice versa. Therefore, if there are eight sequence levels and level 5 is the trigger sequence level, then levels 1 through 5 can branch to levels 1 through 5 only, and levels 6 through 8 can branch to levels 6 through 8 only.

You can tell if secondary branch qualifiers have been specified by looking at the Sequence Levels display. Figure 15-22 shows how the display looks with the configuration that was given in figure 15-20. An arrow is drawn out of level 2, indicating that branching originates from that level, and an arrow is drawn to level 4 to indicate that a branch is going to that level.

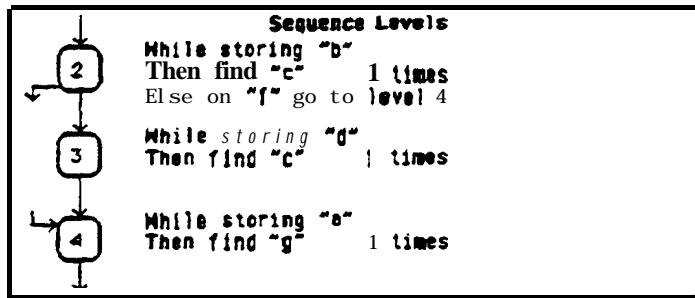


Figure 15-22. Branching Between Sequence Levels

Each sequence level can branch to only one level through a secondary branching qualifier. However, the number of times to which a level can be branched is limited only by the number of levels present. A level can have only one arrow pointing away from it, but it can have two pointing to it if more than one other level is branching to it. An example of this is shown in the figure below. The arrow with two tails indicates that a level above and a level below branch to this level.

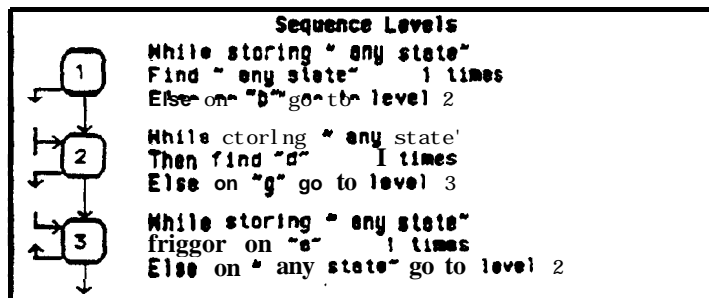


Figure 15-23. Multiple Branching Between Levels

count The count field allows you to place tags on states so you can count them. Counting cuts the acquisition memory in half from 1k to 512 and the maximum clock rate is reduced to 16.67 MHz.

Note 

Count (State Trace menu) is turned off when "Clock Period" is set to < 60 ns in the State Format Specification menu since the clock rate is greater than 16.67 MHz. If you select Count, the clock period automatically changes to > 60 ns.




Figure 15-24. Count Pop-Up Menu

Selecting this field gives you the following pop-up menu.

Off

If you select Off, the states are not counted in the next measurement.

Time

If you select Time counting, the time between stored states is measured and displayed (after the next run) in the State Listing under the label Time. The time displayed can be either relative to the previous state or to the trigger. The maximum time between states is 48 hours.

An example of a state listing with time tagging relative to the previous state is shown in figure 15-25.

8000STATE - State Listing		
Markers <input type="checkbox"/> Off		
Label	DATA	Time
State	Hex	Rel
-0007	00FF	1.24 ns
-0006	6730	
-0005	4BE7	1.26 ns
-0004	4E75	1.72 ns
-0003	3000	1.26 ns
-0002	0000	
-0001	8930	1.24 ns
00000	00FF	1.24 ns
+0001	67FB	1.24 ns
+0002		1.26 ns
+0003	803C	1.24 ns
+0004	61FA	1.72 ns
+0005	803C	1.26 ns
+0006	0000	
+0007	8930	
+0008	4EFA	1.24 ns

Figure 15-25. Relative Time Tagging

An example of a state listing with time tagging relative to the trigger is shown below.

8000STATE - State Listing		
Markers <input type="checkbox"/> Off		
Label	DATA	Time
State	Hex	Abs
-0007	00FF	-9.24 ns
-0006	6730	-7.96 ns
-0005	4BE7	-6.72 ns
-0004	4E75	-5.00 ns
-0003	3000	-3.72 ns
-0002	0000	-2.48 ns
-0001	8930	-1.24 ns
00000	803C	0 ns
+0001	00FF	1.24 ns
+0002	67FB	2.52 ns
+0003	803C	3.76 ns
+0004	61FA	5.00 ns
+0005	803C	6.24 ns
+0006	0000	7.48 ns
+0007	8930	8.72 ns
+0008	4EFA	10.00 ns
+0009		11.24 ns


Figure 15-26. Absolute Time Tagging

States

State tagging counts the number of qualified states between each stored state. If you select this option, you will see a qualifier pop-up menu like that shown in figure 15-2. You select the qualifier for the state that you want to count.

In the State Listing, the state count is displayed (after the next run) under the label States. The count can be relative to the previous stored state or to the trigger. The maximum count is 4.4×10^{12} .

An example of a state listing with state tagging relative to the previous state is shown below.

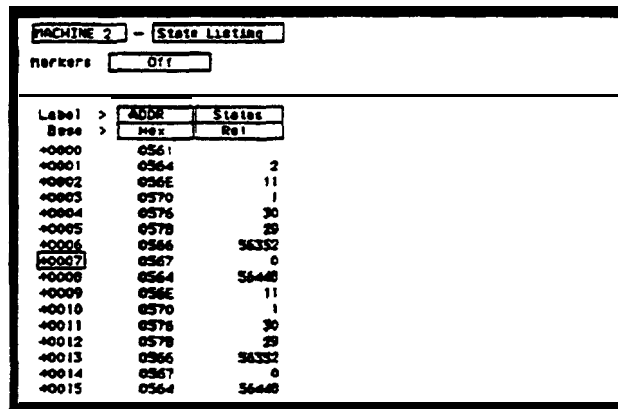

The screenshot shows a window titled "MACHINE 2 - State Listing". At the top, there is a "Markers" button set to "Off". Below this is a table with the following data:

Label >	ADDR	States
Base >	Hex	Rel
+0000	0561	
+0001	0564	2
+0002	056E	11
+0003	0570	1
+0004	0576	30
+0005	0578	29
+0006	0586	36332
+0007	0587	0
+0008	0564	56448
+0009	058E	11
+0010	0570	1
+0011	0578	30
+0012	0578	29
+0013	0586	36332
+0014	0587	0
+0015	0564	56448


Figure 15-27. Relative State Tagging

An example of a state listing with state tagging relative to the trigger is shown below.

Label	ADDR		State
	Hex	Adr	
0000	0561		0
0001	0564		2
0002	056E		13
0003	0570		14
0004	0576		44
0005	0578		73
0006	0566	56425	
0007	0567	56425	
0008	0564	112873	
0009	056E	112884	
0010	0570	11288E	
0011	0576	112915	
0012	0578	112944	
0013	0566	188296	
0014	0567	188296	
0015	0564	225744	

Figure 15-28. Absolute State Tagging

Prestore Restore allows you to store two qualified states before each state that is stored. There is only one qualifier that enables prestore for each sequence level. If you select this field, you will see a pop-up with the options Off and On. Selecting On gives you a qualifier pop-up menu like that in figure 15-2, from which you choose the pattern range or combination of patterns and ranges that you want to prestore.

Note  Prestore is only available when clock period is > 60 ns. If you select Prestore, the clock period automatically changes to > 60ns if it was previously set to < 60 ns.

During a measurement, the state analyzer stores in prestore memory occurrences of the states you specify for prestore. A maximum of two occurrences can be stored. If there are more than two occurrences previous ones are pushed out. When the analyzer finds a state that has been specified for storage, the prestore states are pushed on top of the stored state in memory and are displayed in the State Listing.

Qualifier and Pattern Fields

The **qualifier and pattern fields** appear at the bottom of the State Trace Specification menu. They allow you to specify **patterns** for the **qualifiers** that are used in the **sequence** levels.




Figure 15-29. Qualifier and Pattern Fields

Label The Label fields display the labels that you specified in the State Format Specification menu. The labels appear in the or&r that you specified them; however, you can change the order. Select one of the label fields and you will see a pop-up menu with all the labels. Decide which label you want to appear in the label field and select that label. The label that was there previously switches positions with the label you selected from the pop-up.

Base The base fields allow you to specify the numeric base in which you want to define a pattern for a label. The base fields also let you use a symbol that was specified in the State Symbol Table for the pattern. Each label has its own base defined separately from the other labels. If you select one of the base fields, you will see the following pop-up menu. Decide which base you want to define your pattern in and select that option





Figure 15-30. Numeric Base Pop-Up Menu

One of the options in the Base pop-up is ASCII . It allows you to see the ASCII characters that are represented by the pattern you specify in the pattern fields.

Note 

You cannot define ASCII characters directly. You must first define the pattern in one of the other numeric bases; then you can switch the base to ASCII to see the ASCII characters.

The Symbol option in the Base pop-up allows you to use a symbol that has been specified in the State Symbol Tables as a pattern. In the pattern fields you specify the symbols you want to use.

Qualifier Field If you select the qualifier field, you will see the following pop-up menu.




Figure 15-31. Qualifier Field Pop-Up Menu

Patterns

The pattern recognizers are in two groups of four: a-d and e-h. If you select one of these two options, the qualifier field will contain only those pattern recognizers. For instance, the qualifier field in figure 15-29 contains only the recognizers a-d.

Ranges

If you select the range option, the qualifier and pattern fields look similar to that shown below.

Label >	<input type="text" value="A"/>
Base >	<input type="text" value="Hex"/>
<input type="text" value="Range"/>	
lower	<input type="text" value="0000"/>
upper	<input type="text" value="FFFF"/>

Figure 15-32. Flange Qualifier and Pattern Fields

Only one range can be defined, and it can be defined over only one label, hence over only 32 channels. The channels don't have to be adjacent to each other. The logic analyzer selects the label over which the range will be defined by looking at the labels in order and choosing the first one that has channels assigned under only two pods. A label that contains channels from more than two pods cannot be selected for range definition. If all the labels have channels assigned under more than two pods, the range option is not offered in the qualifier field pop-up menu. However, in the HP 1651B, the range option will always be offered since the analyzer has only two pods.

Pattern Fields

The pattern fields allow you to specify the states that you want the state analyzer to search for and store. Each label has its own pattern field that you use to specify a pattern for that label (if you are defining a pattern for a pattern recognizer).

During a run, the state analyzer looks for a specified pattern in the data. When it finds the pattern, it either stores the state or states or it triggers, depending on the step that the sequencer is on.

State Listing Menu

Introduction

This chapter describes the State Listing menus and how to interpret it. It also tells you how to use the fields to manipulate the displayed data so you can find your measurement answers. The state Listing menu is the display menu of the state analyzer.

There are two different areas of the state listing display, the menu area and the listing area. The menu area is in the top one-fourth of the screen and the listing area is the bottom three-fourths of the screen.

The listing area displays the data that the state analyzer acquires. The data is displayed in a listing format as shown below.

Label >	Addr	Data	Time
Base >	Hex	Hex	RPI
-0007	0080CA	00FF	1.24 us
-0006	0080CC	6730	1.28 us
-0005	0080CE	40E7	1.24 us
-0004	0080FE	4E75	1.72 us
-0003	008000	3000	1.28 us
-0002	0004F4	0000	1.24 us
-0001	0004F6	0030	1.24 us
00000	008030	803C	1.24 us
+0001	008032	00FF	1.24 us
+0002	008034	67F8	1.28 us
+0003	008036	803C	1.24 us
+0004	00803E	61FA	1.72 us
+0005	008030	803C	1.28 us
+0006	0004F4	0000	1.86 us
+0007	0004F6	0030	1.82 us
+0008	00802A	4EFA	1.24 us

Figure 181. State listing Menu

This listing display shows you 16 of the possible 1024 lines of data at one time. You can use the ROLL keys and the KNOB to roll the listing to the lines of interest.

The **column** of numbers at the far left represents the **location** of the **acquired** data in the state **analyzer's** memory. The trigger state **is** always 0000. **At the vertical center of this column you will see a box containing** a number. The box is used to quickly select **another location** in the state **listing**. The **rest** of the **columns** (except the **Time/States** column) represent the data acquired **by the state analyzer**. The data is grouped by label and **displayed** in the **number** base you have **selected** (hexadecimal is the default base).

When the **Time** or States option is selected in the **Count field (State Trace Specification Menu)**, the **acquired** data will be displayed with **time or state tags**.

The **Time column** displays either the **Rel(ative)** time (time from one state to the next) or **Abs(olute) time** (time from each state **to the trigger**).

The States **column** displays the number of qualified states **Rel(ative)** to the previously stored state or the trigger (absolute).

Accessing the State Listing Menu

The **State Listing Menu** is accessed by pressing the **DISPLAY** key on the front panel when the state **analyzer** is on. It **will** automatically be displayed **when** you press **RUN**. If the Timing Waveforms is displayed when you press the **DISPLAY** key, **you will** have to **switch analyzers**. This is not a problem, it merely indicates **that** you were in the timing **analyzer or you had performed an action to the timing analyzer in the System Configuration Menu**.

State listing Menu Fields

The menu area contains fields that allow you to change the display parameters, place markers, and display listing measurement parameters.



Figure 16-2. State Listing Menu Fields

Markers The Markers field allows you to specify how the X and O markers will be positioned on the state listing. The State Trace Specifications menu options are:

If Count in the State Trace menu is Off the marker options are:

- off
- Pattern

If Count in the State Trace menu is set to Time the marker options are:

- Off
- Pattern
- Time
- Statistics

If Count in the State Trace menu is set to State the marker options are:

- □××
- Pattern
- State

Markers Off When the markers are off they are not displayed, but are still placed at the specified points in the data. If Stop measurement is on and the Stop measurement criteria are present in the data, the measurement will stop even though the markers are off.

Markers Patterns When the markers are set to patterns, you can specify patterns on which the logic analyzer will place the markers. You can also specify how many occurrences of each marker pattern the logic analyzer looks for. This use of the markers allows you to find a specific pattern for each label in the acquired data.




Figure 16-3. Markers Set to Patterns

Patterns for each marker (X and O) can be specified. They can be specified for both markers in each label. The logic analyzer searches for the logical "and" of patterns in all labels.

In the Find X (O)-pattern 0 from Trigger field you specify how many occurrences of the marked pattern from a reference point you want the logic analyzer to search for. The reference points are:

- Trigger
- Start (of a trace)
- X Marker (only available in 0 marker pattern specification)




Figure 164. Search Reference Pop-Up Menu

Stop Measurement. Another feature of markers set to patterns is Stop Measurement. You can specify either stop measurement when X-O is or Compare is . The options for X-O are: **Less than**, **Greater than**, **In range**, **Not in range**. The options for Compare are: **Equal** and **Not Equal** (see **figure 16-5**).

Figure 16-5. Markers **Patterns** Pop-Up *Menu*

With this feature you can use the logic analyzer to look for a **specified** time or **range of time** between the marked patterns and to stop **acquiring** data when it finds this time between markers. The X marker must precede the 0 **marker**.

Also available is Store exception to disk which allows you to specify a **file on the disk that exceptions can be stored in. The default filename is EXCEPTION.** When the trace mode is repetitive and Store exception to disk is on, the following process takes place: **data is acquired until the stop criteria is met, data acquisition will stop, data in the acquisition memory will be stored on the disk, and data acquisition will resume when the data is stored. This process continues until the disk is full. The data is stored in the same file name; however, the last three characters will automatically be replaced with a numerical serial number. For example, EXCEPTION will change to EXCEPT001 the second time memory is stored.**

Note 

The upper and lower range boundaries must not **be** the same value. For **example, if you want to stop a measurement when the X and 0 markers are in range of 200 ns, you should set the range values to 190 ns and 210 ns.** This **eliminates erroneous measurement termination.**

Markers Time When the markers are set to Time, you can place the markers on states in the listing of interest and the logic analyzer will tell you:

- Time X to Trig(ger)
- Time 0 to Trig(ger)
- Time X to 0

To position the markers, move the cursor to the field of the marker you wish to position and press SELECT. A pop-up will appear showing the current time for that marker. Either rotate the KNOB or enter a numeric value from the keypad to change the position of that marker. Pressing SELECT when you are finished positions the marker and closes the pop-up.

68000STATE - State Listing	Time X to Trigger	6.76 us
Markers Time	Time 0 to Trigger	3.76 us
	Time x to 0	-3.00 us

Figure 16-6. Markers Set to Time

The Time X to 0 field will change according to the position of the X and 0 markers. It displays the total time between the states marked by the X and 0 markers.

Markers Statistics When statistics are specified for markers, the logic analyzer will display the:

- Number of total runs
- Number of valid runs (runs where markers were able to be placed on specified patterns)
- Minimum time between the X and 0 markers * Maximum time between the X and 0 markers
- Average time between the X and 0 markers

68000STATE - State Listing	Minimum X-0:	0 s
Markers Statistics	Valid runs:	Maximum X-0:
	1 of 4	Average X-0:
		0 s

Figure 16-7. Markers Set to Statistics

How the statistics will be updated depends on the state trace mode (repetitive or **single**).

In **repetitive**, statistics will be updated each time a valid run occurs until you press STOP. When you press RUN after STOP, the statistics will be cleared and will restart from zero.

In **single**, each time you press RUN an additional valid run will be added to the data and the statistics will be updated. This will continue unless you change the placement of the X and 0 markers between runs.

Pattern ___ Field You use the Pattern ___ field to specify the patterns for the X and 0 markers for each label.

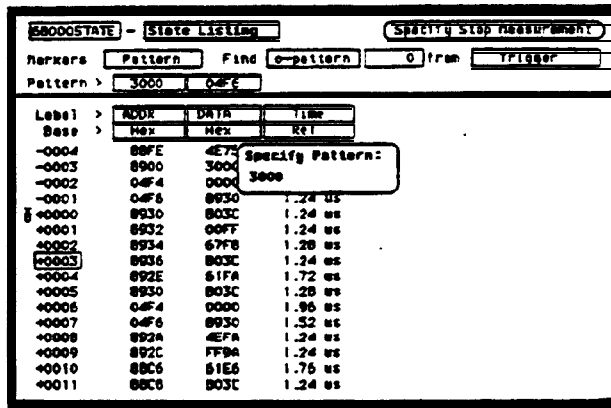


Figure 16-8. Pattern ___ Field Pop-Up Menu

When x-pattern is specified in the Find ___ from ___ field, the pop-ups in the Pattern ___ field allow you to specify a pattern for the X marker in each label.

When the O-pattern is specified, the pop-ups in the Pattern ___ field allow you to specify the patterns for the 0 marker in each label.

State Compare Menu

Introduction

State compare is a software post-processing feature that provides the ability to do a bit by bit comparison between the acquired state data listing and a compare data image. You can view the acquired data and the compare image separately. In addition, there is a separate difference listing that highlights the bits in the acquired data that do not match the corresponding bits in the compare image. Each state machine has its own Compare and Difference listings.

You can use the editing capabilities to modify the compare image. Masking capabilities are provided for you to specify the bits that you do not want to compare. "Don't compare" bits can be specified individually for a given label and state row, or specified by channel across all state rows. A range of states can be selected for a comparison. When a range is selected, only the bits in states on or between the specified boundaries are compared.

The comparison between the acquired state listing data and the compare image data is done relative to the trigger points. This means that the two data records are aligned at the trigger points and then compared bit by bit. Any bits in the acquired data that do not match the bits in the compare image are treated as unequal. The don't compare bits in the compare image are ignored for the comparison.

When a logic analyzer configuration is saved to or loaded from a disk, any valid compare data including the data image, etc. is also saved or loaded

Accessing the Compare Menu

The Compare menu is accessed from the State **Listing menu**. To access the Compare menu place the cursor on the field **State Listing** and press **SELECT**. A pop-up appears with the following options:

- State Listing
- State Waveforms
- State Chart
- State Compare

Place the cursor on State **Compare** and press **SELECT**. The pop-up will close and display the State **Compare** menu

The Compare and Difference Listing Displays

Two menus (or displays) in addition to the normal State Listing, are available for making comparison measurements: the **Compare Listing** and the **Difference Listing**.

The Compare Listing

The **Compare Listing** contains the image (or template) that acquired data is compared to during a comparison measurement. The boundaries of the image (or size of the template) can be controlled by using the **channel** masking and compare range functions described below. Any bits inside the image displayed as "X" have been set to don't compare bits.

The Difference Listing

The **Difference Listing** highlights the entire row with inverse video, if any differences exist, in the acquired data that differs from those in the compare image. In addition, when the base is hexadecimal, octal, or binary, the bit (or digit containing the bit) that differs from the compare image is underlined (see figures 17-2 and 17-3). If the base is **inverse** assembled symbols, the display does not change; however, the stop measurement functions still function.

To display the **Compare Listing** or the **Difference Listing**, place the cursor on the field directly to the right of **Show** in the upper left part of the display and press **SELECT**. The field will toggle between **Compare Listing** and **Difference Listing**.

The **controls** that roll the **listing** in all three **menus**, the normal **State Listing**, the **Compare Listing**, and the **Difference Listing** are synchronized unless the **number** of pre-trigger states differ between the **Compare listing** and the **acquired data**. This means that when you **change the current row position in the Difference Listing**, the **logic analyzer** automatically Updates the current row in the acquired **State Listing**, **Compare Listing** and **vice-versa**.

If the three listings are synchronized and you re-acquire **data**, the **Compare Listing** may have a **different number** of **pre-trigger** states depending on the state trace trigger criteria. The **Compare Listing** can be **resynchronized** to the **State and Difference Listings** (if different) by **entering the desired state (acquisition memory) location** from the front-panel keypad.

This allows you to **view corresponding** areas of the **two** lists, to **cross check the alignment**, and **analyze the bits that do not match**.

Since **time tags** are not required to perform the compare, they do not appear in either the **compare image** or **difference displays**. However, **correlation** is possible since the displays are locked together.

To move between the **State Listing** and **Compare Listing** in the HP 1650B/51B, select the field directly to the right of **Show** in the upper left part of the screen and press **SELECT**. This field toggles between **Compare Listing** and **Difference Listing**.

Creating a Compare Image

An initial compare image can be generated by copying acquired data into the compare image buffer. When you place the cursor on the **Copy Trace to Compare** field in the **Compare Listing** menu a pop-up appears with the options **Cancel** and **Continue**!. If the **Continue** is selected, the contents of the acquisition data structure for the current machine are copied to the compare image buffer. The previous compare image is lost if it has not been saved to a disk. If you select **Cancel** the current compare image remains unchanged.

Bit Editing of the Compare Image

Bit editing allows you to modify the values of individual bits in the compare image or specify them as don't compare bits. The bit editing fields are located in the center of the Compare Listing display to the right of the listing number field (see figure 17-1). A bit editing field exists for every label in the display unless the label's base is ASCII or inverse assembled symbols. You can access any data in the Compare Listing by rolling the desired row vertically until it is located in the bit editing field for that label (column).

When you select one of the bit editing fields a pop-up appears in which you enter your desired pattern or don't compare for each bit.

The screenshot shows a terminal window titled "BOBS - State Compare" with a "Specify Stop Measurement" button. Below the title bar are three buttons: "Compare Listing", "Copy Trace to Compare", and "Full Compare". A "Next" field is present. The main display is a table with columns "Label", "ADDR", "DATA", and "STAT". The "ADDR" column has a sub-header "Hex", and the "DATA" and "STAT" columns also have sub-headers "Hex". The table contains rows of data with addresses from +0065 to +0060. A pop-up window titled "Specify Pattern:" is overlaid on the table, showing the text "Specify Pattern:" and "T82F".

Label	ADDR	DATA	STAT
Base	Hex	Hex	Hex
+0065	0404	03	
+0066	0404	02	
+0067	0404	03	
+0068	0404	02	2
+0069	0404	03	3
+0070	0404	02	2
+0071	0404	03	3
+0072	0404	02	2
+0073	0404	03	3
+0074	0404	02	2
+0075	0404	03	3
+0076	0404	02	2
+0077	0404	03	3
+0078	0404	02	2
+0079	0404	03	3
+0080	0404	02	2

Figure 17-1. Bit Editing Fields

Masking Channels in the Compare Image

The channel masking function allows you to specify a bit, or bits in each label that you do not want compared. This causes the corresponding bits in all states to be ignored in the comparison. The compare data image itself remains unchanged on the display. The Mask fields are directly above the label and base fields at the top of both the Compare and Difference listings (see figure 17-2). When you select one of these fields a pop-up appears in which you specify which channels are to be compared and which channels are to be masked. A "." (period) indicates a don't compare mask for that channel and an "*" (asterisk) indicates that channel is to be compared.

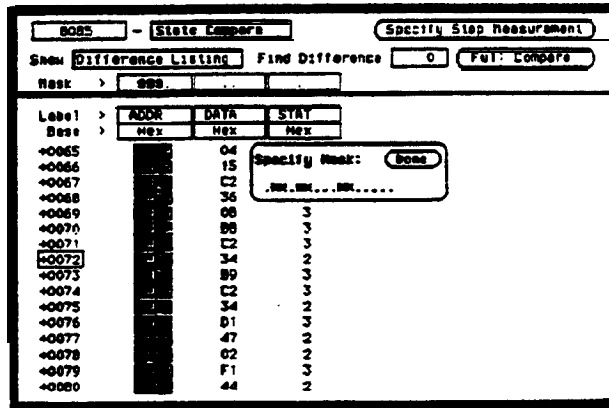


Figure 17-2. Bit Masking Fields

Specifying a Compare Range

The Compare Range function allows you to define a subset of the total number of states in the compare image to be used in the comparison. The range is specified by setting start and stop boundaries. Only bits in states (lines) on or between the boundaries are compared against the acquired data.

The Compare mode is accessed by selecting the Full Compare/Partial Compare field in either the Compare or Difference listing menus. When selected, a pop-up appears in which you select either the Full or Partial option. When you select the Partial option, fields for setting the start state and stop state values appear (see figure 17-3).

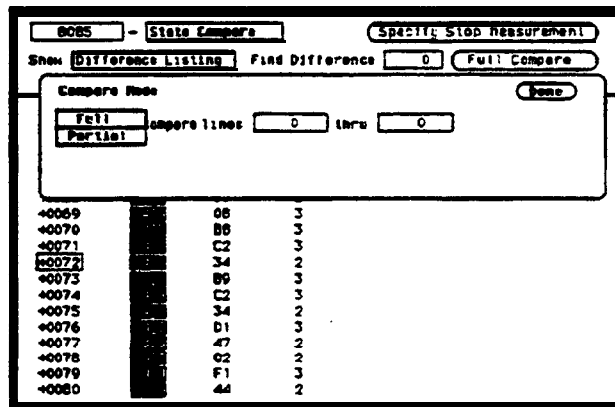


Figure 17-3. Compare Full/Compare Partial Field

Repetitive Comparisons with a Stop Condition

When you do a comparison in the repetitive trace mode, a stop condition may be specified. The stop condition is either Stop Measurement when Compare is Equal or Not Equal. In the case of Equal, bits in the compare image must match the corresponding bits in the acquired data image for the stop condition to be a true. In the case of Not Equal, a mismatch on a single bit will cause the stop condition to be true. When stop conditions are specified in two analyzers, both analyzers stop when the stop condition of either analyzer is satisfied. It is an OR function.

You access the stop measurement function by selecting the Specify Stop Measurement field in either the Compare or Difference Listing menus. When you select this field, the Stop Measurement Parameters pop-up appears (see figure 17-4). The first field in this pop-up, just to the right of Stop measurement contains either Off, X-O or Compare.

When this field is selected, a pop-up appears in which you select Compare. When you select the Compare option, you can access and select either the Equal or Not Equal option in the next field to the right.

+0069	043A	08	3
+0070	043B	08	3
+0071	043C	C2	3
+0072	043D	34	2
+0073	043F	89	3
+0074	0440	C2	3
+0075	0441	34	2
+0076	0443	D1	3
+0077	0886	47	2
+0078	0887	02	2
+0079	0444	F1	3
+0080	088B	44	2

Figure 17-4. Specify Stop Measurement Field

Also available is Store exception to disk which allows you to specify a file on the disk that exceptions can be stored in. The default filename is EXCEPTION.

When the trace mode is repetitive and Store exception to disk is on, the following process takes place: data is acquired until the stop criteria is met, data acquisition will stop, data in the acquisition memory will be stored on the disk, and data acquisition will resume when the data is stored. This process continues until the disk is full. The data is stored in the same file name; however, the last three characters will automatically be replaced with a numerical serial number. For example, EXCEPTION will change to EXCEPT001 the second time memory is stored.

Note 

You may also specify a stop measurement based on time between the X and O markers in the Compare or Difference Listing menus. This is available only when Count is set to Time in the State Trace menu. If the Stop Measurement is set to run until Compare Equal or Compare Not Equal in the Compare or Difference Listings, the Stop Measurement on time X to O will change to run until Compare Equal or Compare Not Equal in the other state display menus (i.e. State Listing).

Locating Mismatches In the Difference Listing

The Find Difference feature allows you to easily locate any patterns that did not match in the last comparison. Occurrences of differences are found in numerical ascending order from the start of the listing. The first occurrence of an error has the numerical value of one.

This feature is controlled by the Find Difference ___ field in the Difference Listing menu. When you select this field an Integer Entry pop-up appears in which you enter a number indicating which difference you want to find. The listing is then scanned sequentially until the specified occurrence is found and rolled into view.

Saving Compare Images

When you save a logic analyzer configuration to a disk, the compare images for both state analyzers are saved with it. The compare data is compacted to conserve disk space. Likewise, when you load a configuration from disk, valid compare data will also be loaded.

State Chart Menu

Introduction

The **State Chart Menu** allows you to build X-Y plots of label activity using state data. The Y-axis **always** represents data values for a specified **label**. You can **select** whether the X-axis represents states (ie. **rows in the State List**) or the **data values** for another label. You can **scale** both the axes to **selectively** view data of interest. An **accumulate** mode is available that allows the chart display to build up over several runs. When State is selected for the X-axis, X & 0 markers are **available which allows the current sample (state or time) relative to trace point to be** displayed. Marker placement is **synchronized** with the normal State Listing.

Accessing the State Chart Menu

The Chart menu is accessed from the State Listing **menu**. To **access** the **Chart** menu place the cursor on the field State Listing and press **SELECT**. A **pop-up** appears **with the following options**:

- **State Listing**
- **State Waveforms**
- **State Chart**
- **State Compare**

Place the **cursor** on State Chart and press **SELECT**. The pop-up **will close** and display the State Chart menu.

Selecting the Axes for the Chart

When using the State **Chart** display, you **should** first select what data you want plotted on each **axis**. Assigning a label to the vertical axis of the **chart** is accomplished by positioning **the** cursor on the Y-axis Label field in the menu. **When selected**, a pop up appears **in** which you select one of the **labels** that were **defined** in the State **Format Specification** Menu. The X-axis assignment field, toggles between State and **Label** **when** selected. When label is selected, a third field appears to the right of **Label that pops up when selected in which you select** one of the defined state labels.

Scaling the Axes

Either axis of the X - Y chart can be scaled by using the associated vertical or horizontal min (minimum) or max (maximum) value fields. When selected, a Specify Number pop up appears in which you specify the actual minimum and maximum values that will be displayed on the chart.

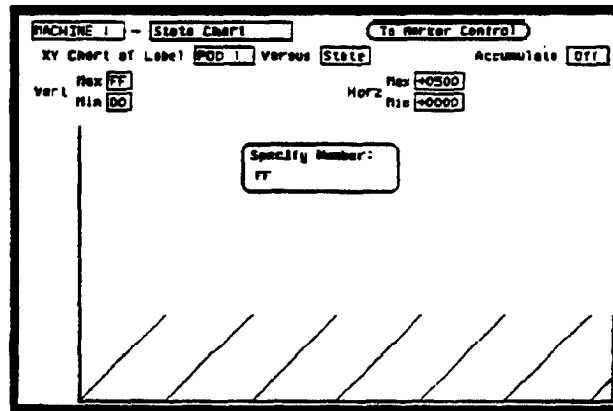


Figure 18-1. Axis Scaling Pop-up Menu

When **State** is selected for the X-axis, state acquisition memory locations are plotted on the X-axis. The minimum and maximum values can range from -1023 to +1023 depending on the trace point location. The minimum and maximum values for labels can range from 00000000H to FFFFFFFFH (0 to $2^{32}-1$) regardless of axis, since labels are restricted to 32 bits.

The Label Value vs. States Chart

The Label Value versus State chart is a plot of label activity versus the memory location in which the label data is stored. The label value is plotted against successive analyzer memory locations. For example, in the following figure, label activity of POD 1 is plotted on the Y axis and the memory locations (State) are plotted on the X axis.

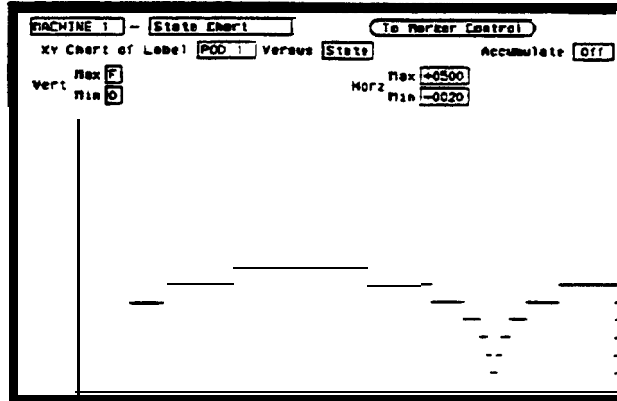


Figure 18-2. label vs. State Chart

The Label Value v s . Label Value Chart

When labels are assigned to both axis, the chart shows how one label varies in relation to the other for a particular state trace record. Label values are always plotted in **ascending** order from the bottom to the top of the chart and in **ascending order from left to right across the chart**. Plotting a label against itself will result in a diagonal line from the lower left to upper right corner. X & O markers are disabled when operating in this mode.

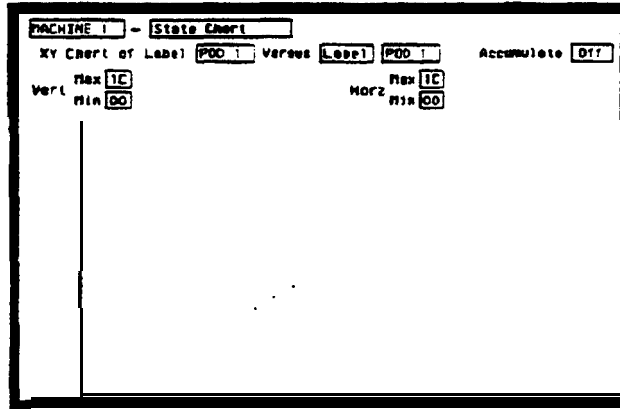


Figure 18-3. Label vs. Label chart

X & O Markers and Readouts for Chart

When State is specified for the X-axis, X & O markers are available which can be moved horizontally. The markers are synchronized with the X and O markers in the normal State Listing.

To select the marker mode for Chart (if it is not presently displayed), place the cursor on the To Marker Control field and press SELECT. This field will toggle to To Range Control and the marker fields will be displayed (see figure 18-4).

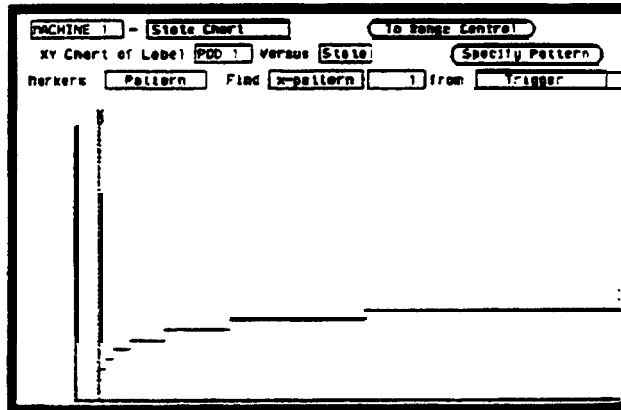


Figure 18-4. Marker Fields

When a marker is positioned in the State Chart menu, it is also positioned in the State Listing menu and vice-versa. The Chart marker operation is identical to the markers in the State Listing menu (see chapter 16).

Marker Options The marker options in the state **Chart** menu depend on what **Count** is set to in the **State Listing** menu.

When **Count** is set to **Off** the **Chart** markers can be set to:

- □××
- PatteHl

When **Count** is set to **Time** the **Chart** markers can be set to:

- off
- Pattern
- ※)(
- Statistics

When **Count** is set to **States** the **Chart** markers can be set to:

- Pattern
- states

State Waveforms Menu

Introduction

The State **Waveforms Menu** allows you to view state data in the form of waveforms **identified** by label name and bit number. Up to **24** waveforms can be displayed simultaneously. Only state data from the **current** state **machine** can be displayed as waveforms **in** the State **Waveforms menu**.

The presentation and user interface is generally the same as the **Timing** Waveform menu, except the **X-axis** of the state waveform display represents only samples, or states instead of time (seconds). **This** is true regardless of whether Count (in **the** State Trace menu) is set to **Time** or Off. As a result, the horizontal axis of the display **is** scaled by **States/Div** and Delay in terms of samples from trigger. Marker features **are the same as for State List in that Time or States will only be** available when Count is set to **Time** or States. The **Sample** Rate display is not available in State Waveform **even** when markers are off.

Accessing the State Waveforms Menu

The State **Waveforms menu** is accessed from the State Listing **menu**. To access the State **Waveforms** menu **place** the **cursor** on the State Listing field and press SELECT. A pop-up appears **with** the **following** options

- **State Listing**
- State Waveforms
- **State Chart**
- **State Compare**

Place the **cursor** on State Waveforms and press SELECT. The **pop-up** will close and display the State Waveforms **menu**.

Selecting a Waveform

You can display up to 24 waveform on screen at one time. Each waveform is a representation of a predefined label. To select a waveform, place the cursor on a label name on the left side of the display and press SELECT. A pop-up appears in which you:

- Insert waveforms
- Turn on waveforms
- Modify waveforms (waveformlabels)
- Turn off waveforms
- Delete waveforms

Just to the right of each label name is a two-digit number or the word "all." The number indicates which bit of the label the waveform represents; or, all the bits of the label when "all" is displayed (see figure 19-1).

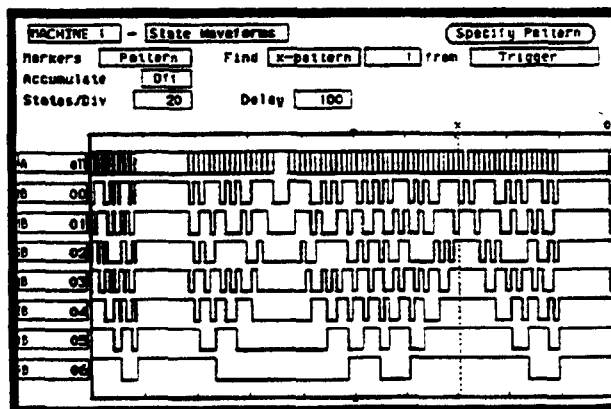


Figure 19-1. State Waveforms Menu

In the above figure, label A has "all" specified displaying all the bits overlaid in a single waveform. Label B however, has seven of its bits displayed individually (bits 0 through 6).

Replacing Waveforms

You can **replace** a **currently displayed** waveform (label) with another one of the **predefined** waveforms (**labels**). To replace one waveform with another, **place** the cursor **on** the waveform you wish to replace and press **SELECT**. A **pop-up** appears in which you select **Modify Waveform** as **shown** in the following figure.

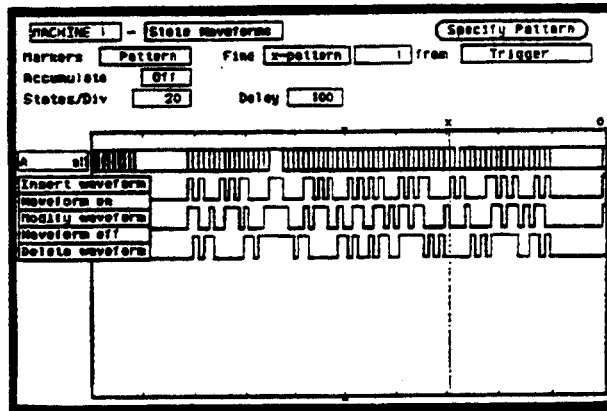


Figure 19-2. Waveform Selection Pop-up Menu

Another pop-up appears in which you select the waveform (label) you wish to display (see figure 19-3). When you place the cursor on the new waveform (label) and press SELECT the new waveform replaces the old waveform.

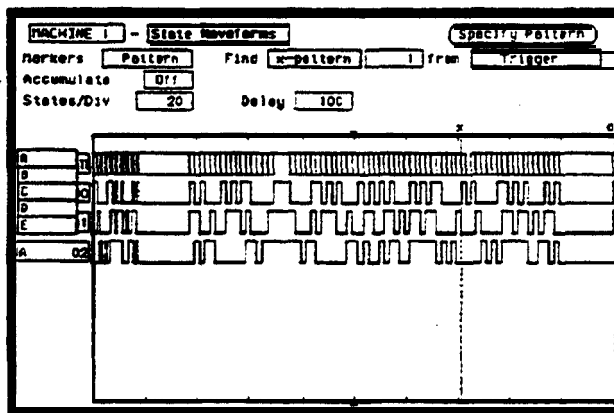


Figure 19-3. Available Waveforms Pop-up Menu

Deleting Waveforms

You can delete any of the currently displayed waveforms by placing the cursor on the waveform you wish to delete and pressing SELECT. When the pop-up appears place the cursor on **Delete** waveform and press SELECT.

Selecting States per Division

You can specify the states per division by placing the cursor on the field just to the right of **States/Div**, pressing SELECT, and either entering the **number** of states per division with the keypad or the knob. The range is from 1 to 1024 per division.

Delay from Trigger

You can **specify** the delay from trigger by **specifying** the number of states from the trigger. The delay will **affect only** the position of the State Waveforms display. it does not affect data **acquisition**. The **minimum** is - 1024 and the maximum is 1024 independent of trace position in the record Delay is not limited to the window **containing** data.

State Waveform Display Features

The waveform display features of the State Waveform menu are the same as the Timing Waveform menu with regard to:

- low levels (below threshold) are represented by darker **line**
- dotted **lines** representing the X and 0 markers
- inverted triangle **representing** the trigger **point**
- **Accumulate Mode**
- **graticule** frame with 10 horizontal divisions

X and 0 Markers for State Waveform

Markers can be placed on the waveform display by **specifying** the **number** of states from trigger or start in the case of the X marker or number of states from **either** the trigger, start, or X marker in the case of the 0 marker.

Markers can be **automatically** placed on the waveform by searching for specific patterns assigned to each marker.

The X and 0 marker operation is identical to the marker operation in the **Timing Waveform Menu** (see chapter 11).

State Analyzer Measurement Example

Introduction

In this chapter you will learn how to use the state analyzer by setting up the logic analyzer to make a simple state measurement. We give you the measurement results as actually measured by the logic analyzer, since you may not have the same circuit available.

The exercise in this chapter is organized in a task format. The tasks are in the same order you will most likely use them once you become experienced. The steps in this format are both numbered and lettered. The numbered steps state the step objective. The lettered steps explain how to accomplish each step objective. There is also an example of each menu after it has been properly set up.

How you use the steps depends on how much you remember from chapters 1 through 4 of the *Getting Started Guide*. If you can set up each menu by just looking at the menu picture, go ahead and do so. If you need a reminder of what steps to perform, follow the numbered steps. If you still need more information about 'how,' use the lettered steps.

When you have finished configuring the logic analyzer for this exercise, you can load a file from the operating system disc. This file configures the logic analyzer the same way it is configured for this exercise. It also loads the same data acquired for this exercise so you can see what it looks like on screen.

In order to learn how to configure the logic analyzer, we recommend that you follow the exercise to "Acquiring the Data" before loading the file from the disc.

You can also compare your configuration with the one on the disc by printing it (if you have a printer) or making notes before you load the file.

Problem Solving with the State Analyzer

In this example assume you have designed a microprocessor controlled circuit. You have completed the hardware, and the software designer has completed the software and programmed the ROM (read-only memory). When you turn your circuit on for the first time, your circuit doesn't work properly. You have checked the power supply voltages and the system clock and they are working properly.

Since the circuit has never worked before, you and the software engineer aren't sure if it is a hardware or software problem. You need to do some testing to find a solution

What Am I Going to Measure?

You decide to start where the microprocessor starts when power is applied. We will describe a 68000 microprocessor; however, every processor has similar start-up routines.

When you power up a 68000 microprocessor, it is held in reset for a specific length of time before it starts doing anything to stabilize the power supplies. The time the microprocessor is held in reset ensures stable levels (states) on all the devices and buses in your circuit. When this reset period has ended, the 68000 performs a specific routine called fetching the reset vector.

The first thing you check is the time the microprocessor is held in reset. You find the time is correct. The next thing to check is whether the microprocessor fetches the reset vector properly.

The steps of the 68000 reset vector fetch are:

1. Set the stack pointer to a location you specify, which is in ROM at address locations 0 and 2
2. Find the first address location in memory where the microprocessor fetches its first instruction. This is also specified by you and stored in ROM at address locations 4 and 6.

What you decide to find out **is**:

1. What ROM address does the **microprocessor** look at for the **location** of the stack pointer, and **what** is the stack pointer **location** stored in ROM?
2. **What ROM** address **does** the microprocessor look at for the address where its **first** instruction is stored in ROM, and is the **instruction correct**?
3. Does the microprocessor then go to the address where its first **instruction** is stored?
4. **Is the** executable **instruction** stored in **the** first instruction location correct?

Your **measurement, then**, requires **verification** of the sequential addresses the **microprocessor** looks **at**, and of the data in ROM at these **addresses**. If the reset vector fetch is correct (**in** this example) you **will** see the **following** list of numbers in HEX (default base) **when** your **measurement** results are displayed.

```
+ 0000 000000 0000
+ 0001 000002 04FC
+ 0002 000004 0000
+ 0003 000006 8048
+ 0004 008048 3E7C
```

This list of numbers will be explained in detail later in this chapter in "The State Listing."

How Do I Configure the Logic Analyzer?

In order to make this state measurement, you must configure the logic analyzer as a state analyzer. By following these steps you will configure Analyzer 1 as the state analyzer.

If you are in the System Configuration menu you are in the right place to get started and you can start with step 2; otherwise, start with step 1.

1. Using the field in the upper left corner of the display, get the System Configuration menu on screen.
 - a. Place the cursor on the field in the upper left corner of the display and press SELECT.
 - b. Place the cursor on System and press SELECT.
2. In the System Configuration menu, change the Analyzer 1 type to State. If Analyzer 1 is already a state analyzer, go on to step 3.
 - a. Place the cursor on the Type: ____ and press SELECT.
 - b. Place the cursor on State and press SELECT.

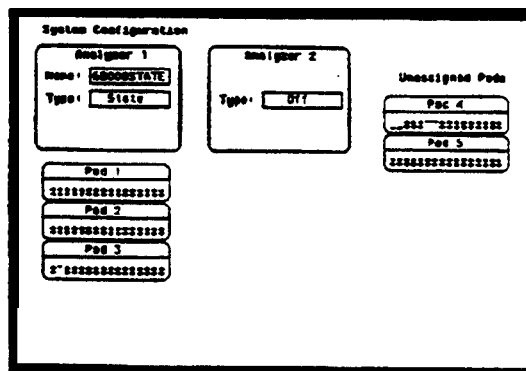


Figure 20-1. System Configuration Menu

3. Name **Analyzer 1** 68000STATE (optional).
 - a. Place the cursor on the **Name: _____** field of **Analyzer 1** and press **SELECT**.
 - b. With the **Alpha Entry** pop-up, change the name to **68000STATE**.
4. Assign pods 1, 2, and 3 to the state analyzer.
 - a. Place the cursor on the **Pod 1** field and press **SELECT**.
 - b. In the **Pod 1** pop-up, place the cursor on **Analyzer 1** and press **SELECT**.
 - c. Repeat steps a and b for pods 2 and 3.

Connecting the Probes

At this point, if you had a target system with a 68000 microprocessor, you would **connect** the **logic** analyzer to your system. **Since** you will be **assigning** labels ADDR and DATA, you hook the probes to your **system accordingly**.

- **Pod 1 probes 0 through 15 to the data bus lines D0 through D15.**
- Pod 2 probes 0 through 15 to the address bus lines **A0** through **A15**.
- Pod 3 probes 0 through 7 to the address bus lines **A16** through **A23**.
- **Pod 1, CLK (J clock) to the address strobe (LAS).**

Activity Indicators

When the logic **analyzer** is connected and your target system is **running**, you will see) in the Pod **1, 2,** and 3 fields of the System Configuration menu. This indicates **which** signal lines are **transitioning**.

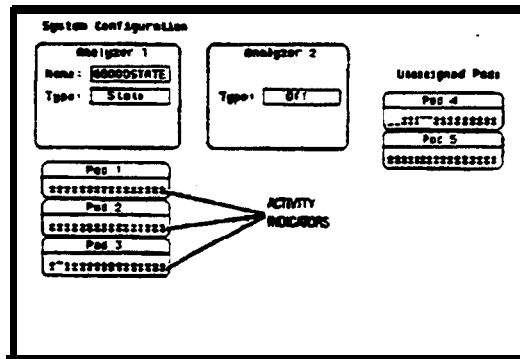


Figure 20-2. Activity Indicators

Configuring the State Analyzer

Now that you have configured the system, you are ready to configure the state analyzer. You will be:

- creating two names (labels) for the input signals
- Assigning the channels connected to the input signals
- Specifying the State (J) clock
- Specifying a trigger condition

L Display the STATE FORMAT SPECIFICATION menu.

a. Press the FORMAT key on the front panel.

2 Name two labels, one ADDR and one DATA

a. Place the cursor on the top field in the label column and press SELECT.

b. Place the cursor on Modify label and press SELECT.

E6000STATE - State Format Specification Specify Symbols

Clock
J

Clock Period > 60 ns

	Pad 3	Pad 2	Pad 1
Activity	TTL	TTL	TTL
Label	Clock	Clock	Clock
Pat	15... 87... 0	15... 87... 0	15... 87... 0

ADDR
DATA
-OFF-
-OFF-
-OFF-
-OFF-
-OFF-
-OFF-
-OFF-
-OFF-

Figure 20-3. State Format Specification Menu

- c. With the Alpha Entry pop-up, change the name of the label to ADDR.
- d. Name the second **label** DATA by repeating steps a through c.

3. Assign Pod 1 bits 0 through 15 to the label DATA.

- a. **Place the cursor on the bit assignment** field below Pod 1 and to the right of DATA and **press** SELECT.
- b. Any combination of bii may **already** be assigned to this pod; however, you will want all **16** bii assigned to the DATA label. **The easiest way to assign is to press the CLEAR ENTRY key to unassign** any assigned bii before you start.
- c. Place the cursor on the period under the **15** in the bit assignment **pop-up and press SELECT. This will place an asterisk in the pop-up** for bit **15**, indicating Pod 1 bit **15** is now assigned to the DATA label. Repeat **this procedure until all** 16 bits have an asterisk **under** each bit number. Place the cursor on Done and press **SELECT** to close the **pop-up**.
- d. Repeat step c for Pod 2 and **the ADDR label** to assign all **16 bits**.
- e. Repeat step c **except you will** assign the lower eight bits (0 - 7) of **Pod 3 to the ADDR label**.

Specifying the J Clock

If you remember from "What's a State Analyzer" in *Feeling Comfortable With Logic Analyzers*, the state analyzer samples the data under the control of an external clock, which is "synchronous" with your circuit under test. Therefore, you must specify which clock probe you will use for your measurement. In this exercise, you will use the J clock, which is accessible through pod L.

1. Select the STATE FORMAT SPECIFICATION menu by pressing the FORMAT key.
2. Set the J Clock to sample on a negative-going edge.
 - a. Place the cursor on the CLOCK field and press SELECT.
 - b. Place the cursor on the box just to the right of J in the pop-up (labeled OFF) and press SELECT.
 - c. Place the cursor on ↓ and press SELECT.
 - d. Place the cursor on Done and press SELECT.

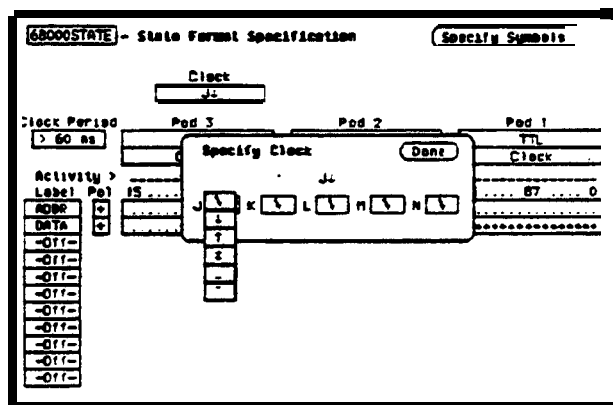


Figure 20-4. Specifying the J Clock

Specifying a Trigger Condition

To capture the data and place the data of **interest** in the center of **the** display of the STATE **LISTING** menu, you need to tell the state **analyzer** when to trigger. Since the first event of interest is address 0000, you need to **tell** the state analyzer to trigger when it detects address 0000 on the **address bus**.

1. Select the STATE **TRACE** SPECIFICATION menu by pressing the TRACE key.
2. Set the trigger so that the state **analyzer** triggers on address 0000. If the Trigger on option is not already a perform steps a through d. If **the option is a skip to step c.**
 - a. Place the **cursor on** the 1 in the Sequence Levels field of **the** menu and press **SELECT**.

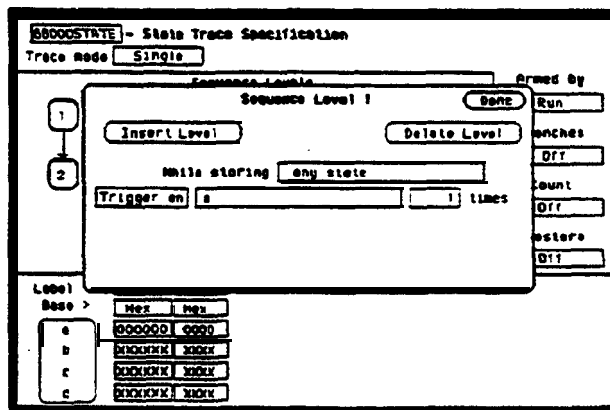


Figure 20-5. State Trace Specification Menu

- b. Place **the** cursor on the **field** to the right of the Trigger on field and press **SELECT**. Another pop-up appears showing you a list of "trigger on" options. Options a through **h** are **qualifiers**. You can assign them a pattern for the bigger specification

- c. Place the cursor on the a option and press SELECT.
- d. Place the cursor on Done in the Sequence Levels pop-up and press SELECT.
- e. Place the cursor on the field to the right of the a under the label ADDR and press SELECT.
- f. With the keypad, press 0 (zero) until there are all zeros in the Specify Pattern: pop-up and then press SELECT.

Your trigger specification now states While storing anystate trigger on "a" once and then store anystate.

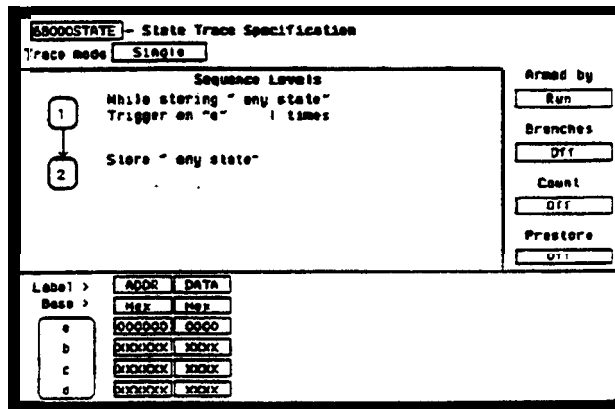



Figure 20-6. State Trace Specification

When the state analyzer is connected to your circuit and is acquiring data, it continuously stores until it sees 0000 on the address bus, then it will store anystate until the analyzer memory is filled.

Acquiring the Data

Since you want to capture the data when the microprocessor sends address 0000 on the bus after power-up, you press the RUN key to arm the state analyzer and then force a reset of your circuit. When the reset cycle ends, the microprocessor should send address 0000 trigger the state analyzer and switch the display to the STATE LISTING menu.

We'll assume this is what happens in this example, since the odds that the microprocessor won't send address 0000 are very low.

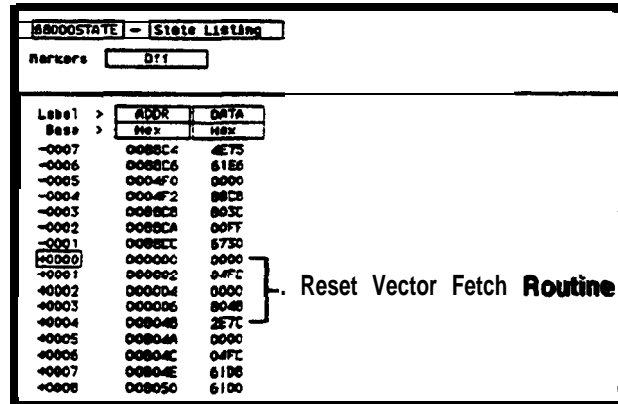


Label	ADDR	DATA
Base	Hex	Hex
-0007	0080C4	4E75
-0006	0080C6	61E6
-0005	0004F0	0000
-0004	0004F2	00C8
-0003	0080C8	003C
-0002	0080CA	00FF
-0001	0080CC	5750
-0000	000000	0000
-0001	000002	04FC
-0002	000004	0000
-0003	000006	8048
-0004	000008	2E7C
-0005	00000A	0000
-0006	00000C	04FC
-0007	00000E	6108
-0008	000010	6100

Figure 20-7. Reset Vector Fetch Routine

Now is the time to load the state measurement demo file from the disc if you wish. The file name is STATEDEMO. Refer to "Load Operation" in chapter 6 if you need a reminder on how to load a file.

The State Listing

The state listing displays three columns of numbers as shown:

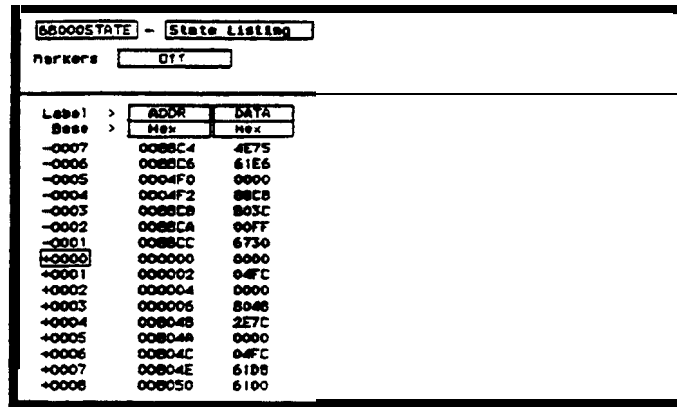

The screenshot shows a terminal window titled "0000STATE - State Listing". Below the title is a "Markers" field with the value "011". The main display area contains a table with the following data:

Label	Base	ADDR	DATA
-0007		008C4	4E75
-0006		008C6	61E6
-0005		000F0	0000
-0004		000F2	80C8
-0003		008C8	803C
-0002		008CA	00FF
-0001		008CC	6730
+0000		00000	0000
+0001		00002	04FC
+0002		00004	0000
+0003		00006	8048
+0004		00008	2E7C
+0005		0000A	0000
+0006		0000C	04FC
+0007		0000E	61D8
+0008		00010	6100

State Locations

Figure 20-8. State Locations

The first column of numbers are the state line number locations as they relate to the trigger point. The trigger state is on line + 0000 in the vertical center of the list area. The negative numbers indicate states occurring before the trigger and the positive numbers indicate states occurring after the trigger.

The second column of numbers are the states (listed in HEX) the state analyzer sees on the address bus. This column is labeled ADDR.

The third column of numbers are the states (listed in HEX) the state analyzer sees on the data bus. This column is labeled DATA.

Finding the Answer

Your answer is now found in the listing of states + 0000 through + 0004.

The 68000 always reads address locations 0, 2, 4, and 6 to find the stack pointer location and memory location for the instruction it fetches after power-up. The 68000 uses **two** words for each of the locations that it is looking for, a high word and a low word. When the software designers program the ROM, they must put the stack pointer location at address **locations 0 and 2. 0 is the high word location and 2 is the low word** location. Siily, the high word of the instruction fetch location must **be in address location 4 and the low word in location 6.**

In order for the 68000 to do this, **the software** design calls for **the** reset vector to:

1. set the stack pointer to 04FC, and

2 read memory address location 8048 for its first instruction fetch.

Therefore, you are interested **in** what is on both the address bus and **the data bus in states 0 through 3.**

You look at the following listing and see that states 0 and 1 do contain address locations 0 and 2 under **the ADDR label**, indicating **the microprocessor** did look at the correct locations for the stack pointer data. You also see **that** the data **contained** in these ROM locations are **0000 and 04FC, which** are correct.

You then look at states 2 **and** 3. You see that the next two **address locations** are 4 and 6, which is correct, and the data **found** at these **locations is 0000 and 8048, which is also correct.**

```
+ 0000 000000 0000
+ 0001 000002 04FC
+ 0002 000004 0000
+ 0003 000006 8048
+ 0004 008048 3E7C
```

So far you have verified that the microprocessor has correctly performed the reset vector search. The next thing you must verify is whether the microprocessor addresses the correct location in ROM that it was instructed to address in state 4 and whether the data is correct in this ROM location. From the listing you see that the address in state 4 is 008048, which is correct, but the instruction found in this location is 2E7C, which is not correct. You have found your problem: incorrect data stored in ROM for the microprocessor's first instruction.

- + 0000 000000 0000 (high word of stack pointer location)
- + 0001 000002 04FC (low word of stack pointer location)
- + 0002 000004 0000 (high word of instruction fetch location)
- + 0003 000006 8048 (low word of instruction fetch location)
- + 0004 008048 2E7C (first microprocessor instruction)

00000STATE - State Listing			
Markers <input type="text" value="DT1"/>			
Label	ADDR	DATA	
Base	Hex	Hex	
-0007	008BC4	4E75	
-0006	008BC5	61E5	
-0005	004FF0	0000	
-0004	004FF2	88C8	
-0003	008BC8	843C	
-0002	008BCA	00FF	
-0001	008BCC	6730	
00000	000000	0000	
+0001	000002	04FC	
+0002	000004	0000	
+0003	000006	8048	
+0004	008048	2E7C	— Incorrect Data
+0005	00804A	0000	
+0006	00804C	04FC	
+0007	00804E	6188	
+0008	008050	6180	

Figure 20-B. Incorrect Data

Summary

You have just learned how **to make** a simple state measurement with the HP **1650B** Logic **Analyzer**. You have:

- **specified a state analyzer**
- learned which probes to **connect**
- **assigned pods 1, 2, and 3**
- **assigned labels**
- **assigned bits**
- specified the J clock
- specified a trigger **condition**
- **acquired the data**
- interpreted the state listing

You have seen how easy it is to use the state **analyzer** to capture the **data** on **the** address and data buses. You can use this same technique to capture and display related data on the microprocessor status control, and various **strobe lines**. You are not limited to using this **technique** on microprocessors. You can use this **technique** any time you need to capture data on multiple lines and need to sample the data relative to a system clock.

Chapter **20** **shows** you how to use the logic **analyzer** as **an interactive** timing and **state analyzer**. You will see a simple measurement **that** shows you both timing waveforms and **state listings** and how **they** are **correlated**.

If you **have an HP 1651B**, you do not have enough **channels** to simultaneously **capture** all the data for a **68000**. But, since you probably aren't working with **16-bit microprocessors**, **this example is still valuable** because it shows you how to make the same kind of measurement on an eight-bit microprocessor.

Mixed Mode Displays

Introduction

This chapter shows you both a timing/state and a state/state mixed mode display. The **detailed** operation of each individual type of display is in their **respective chapters**. Only the **unique** features of the mixed modes displays are given here.

Accessing Mixed Mode Displays

you can access **mixed mode displays when both analyzers are on and Count** is set to The in the State Trace Specification menu. **Mixed mode displays are only available for two state analyzers or one timing and one state analyzer.** To display mixed mode, place the cursor on the field in the upper **left** corner of the display and press SELECT. When the pop-up **appears** you will see **the** Mixed mode option. Place the cursor on **this** option and press **SELECT**. When the pop-up closes, **mixed mode will be** displayed.

Timing/State Mixed Mode Display

When both timing and state analyzers are on you can display both the State Listing and the Timing Waveforms simultaneously as shown.

The data in both parts of the display can be time-correlated as long as Count (State Trace menu) is set to Time.

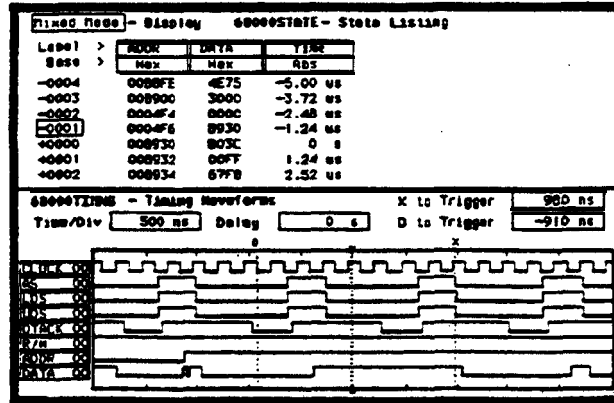


Figure 21-1. Timing/State Mixed Mode Display

The markers for the State Listing and the Timing Waveform in time-correlated Mixed Mode are different from the markers in the individual displays. You will need to place the markers on your points of interest in the time-correlated Mixed Mode even though you have placed them in the individual displays.

**State/State
Mixed Mode
Display**

When two state analyzers are on, the logic analyzer will display both state listings as shown below. Data from state machine 1 is the data with the normal memory location columns filled and with normal black on white video. State machine 2 data is interlaced and displayed in inverse video (white on black). Its memory locations are offset to the right in a column.

To time-correlate data from two state machines, you must set the Count (State Trace menu) for both machines to Time.

Label >	ADDR	DATA	DATA	STATUS	Time	STAT
Base >	Hex	Hex	ASCII	Symbol	Ref	Symbol
+0018	0396	ED			467.4 us	OPCODE FETCH
+0019	0397	78			680 ns	OPCODE FETCH
+0020	8006	E2			920 ns	I/O READ
+0021	03C5	ED			7.24 us	OPCODE FETCH
+0022	03C5	79			680 ns	OPCODE FETCH
+0023	8006	62			920 ns	I/O WRITE
+0024	0396	ED			469.2 us	OPCODE FETCH
+0025	0397	78			640 ns	OPCODE FETCH
+0026	8006	80			920 ns	I/O READ
+0027	03C5	ED			7.26 us	OPCODE FETCH
+0028	03C5	78			640 ns	OPCODE FETCH
+0029	8006	0D			920 ns	I/O WRITE
+0030	0396	ED			464.4 us	OPCODE FETCH

Figure 21-2. Dual-State Machine Mixed Mode Display

The markers for a State/State time-correlated Mixed Mode will be the same as the markers placed in each of the individual State Listings.

Time-Correlated Displays

The HP1650B/51B Logic Analyzers can time-correlate data between the timing analyzer and the state analyzer (see Timing/State Mixed Mode Display) and between two state analyzers (see State/State Mixed Mode Display). In order for the logic analyzer to time-correlate data, the Count in the State Trace menu must be set to Time before you start an acquisition.

The logic analyzer uses a counter to keep track of the time between the triggering of one analyzer and the triggering of the second. It uses this count in the mixed mode displays to reconstruct time-correlated data.

Timing/State Measurement Example

Introduction

In this chapter you will learn how to use the timing and state analyzers interactively by setting up the logic analyzer to make a simple measurement. We give you the measurement results as actually measured by the logic analyzer, since you may not have the same circuit available.

The exercise in this chapter is organized differently than the exercises in the two previous chapters. Since you have already set up both the timing and state analyzers, you should be ready to set them up for this measurement by looking at the menu pictures.

Any new set-ups in this exercise will be explained in task format steps like the previous chapters.

How you use the steps depends on how much you remember from chapters 1 through 4 of the *Getting Started Guide*. If you can set up each menu by just looking at the menu picture, go ahead and do so. If you need a reminder of what steps to perform, follow the numbered steps. If you still need more information about "how," use the lettered steps.

When you have finished configuring the logic analyzer for this exercise, you can load a file from the operating system disk. This file configures the logic analyzer the same way it is configured for this exercise. It also loads the same data acquired for this exercise so you can see what it looks like on screen.

In order to learn how to configure the logic analyzer, we recommend that you follow the exercise to "Acquiring the Data" before loading the file from the disk.

You can also compare your configuration with the one on the disk by printing it (if you have a printer) or making notes before you load the file.

Problem Solving with the Timing/State Analyzer

In this example assume you have designed a microprocessor-controlled circuit. You have completed the hardware, and the software designer has completed the software and programmed the ROM (read-only memory). When you turn your circuit on for the first time, your circuit doesn't work properly. You have checked the power supply voltages and the system clock, and they are working properly.

Since the circuit has never worked before, you and the software engineer aren't sure if it is a hardware or software problem. You need to do some testing to find a solution.

You also notice the circuit fails intermittently. More specifically, it only fails when the microprocessor attempts to address a routine that starts at address 8930.

What Am I Going to Measure?

To see what might be causing the failure, you decide to start where the microprocessor goes to the routine that starts at address 8930. The first thing you check is whether the microprocessor actually addresses address 8930. The next thing you check is whether the code is correct in all the steps in this routine.

Your measurement, then, requires verification of:

- whether the microprocessor addresses location 8930
- whether all the addresses within the routine are correct
- whether all the data at the addresses in the routine are correct

If the routine is correct, the state listing will display:

```
+ 0000 008930 B03C
+ 0001 008932 61FA
+ 0002 008934 67F8
+ 0003 008936 B03C
+ 0004 00892E 61FA
```

How Do I Configure the Logic Analyzer?

In order to make this measurement, you must configure the logic analyzer as a state analyzer because you want to trigger on a specific state (8930). You also want to verify that the addresses and data are correct in the states of this routine.

Configure the logic analyzer so that Analyzer 1 is a state analyzer as shown:

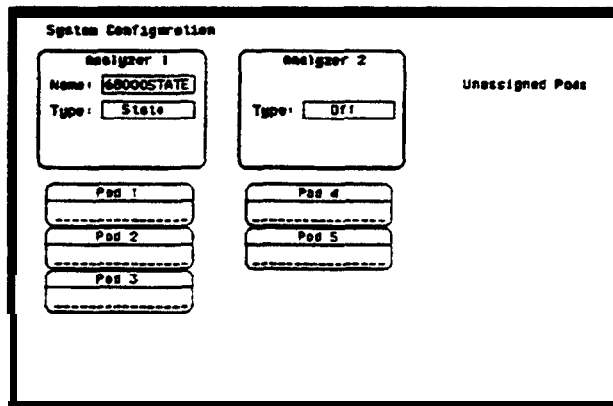


Figure 22-1. System Configuration Menu

Configuring the State Analyzer

Now that you have configured the system, you are ready to configure the state analyzer. Configure the STATE FORMAT SPECIFICATION menu as shown:

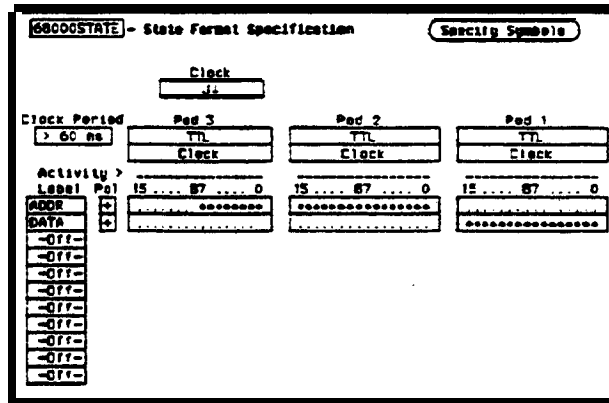


Figure 22-2. State Format Specification Menu

Configure the STATE TRACE SPECIFICATION menu as shown:

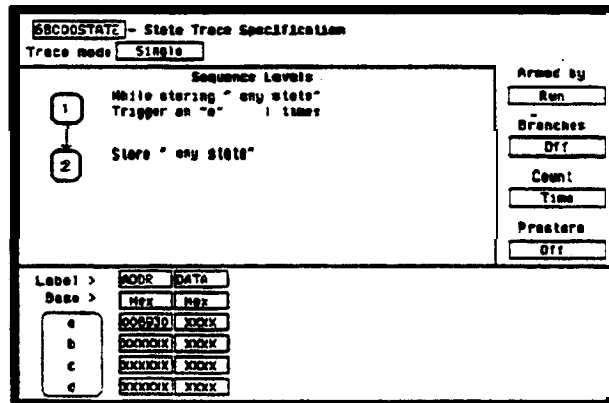


Figure 22-3. State Trace Specification Menu

Connecting the Probes

At this point, if you had a target system with a 68000 microprocessor, you would connect the logic analyzer to your system. Since you will be assigning labels ADDR and DATA, you will hook the probes to your system accordingly.

- Pod 1 probes 0 through 15 to the data bus lines D0 through D15
- Pod 2 probes 0 through 15 to the address bus lines A0 through A15
- Pod 3 probes 0 through 7 to the address bus lines A16 through A23
- Pod 1, UK (J dock) to the address strobe (LAS)

Acquiring the Data

Since you want to capture the data when the microprocessor sends address 8930 on the bus, you press the RUN key to arm the state analyzer. If the microprocessor sends address 8930, it will trigger the state analyzer and switch the display to the STATE LISTING menu.

We'll assume this is what happens in this example.

Finding the Problem

You look at this listing to see what the data is in states + 0000 through + 0004. You know your routine is five states long.

The 68000 does address location 8930, so you know that the routine is addressed. Now you need to compare the state listing with the following correct addresses and data:

```
+ 0000 008930 B03C
+ 0001 008932 61FA
+ 0002 008934 67F8
+ 0003 008936 B03C
+ 0004 00892E 61FA
```

As you compare the state listing (shown below) with the above data you notice the data at address 8932 is incorrect. Now you need to find out why.

Label	Addr	Data
-0007	0088CA	00FF
-0006	0088CC	8730
-0005	0088CE	4E7
-0004	0088FE	4E75
-0003	008900	3000
-0002	0004F4	0000
-0001	0004F6	9530
+0000	008930	B03C
+0001	008932	00FF — Incorrect Data
+0002	008934	67F8
+0003	008936	B03C
+0004	00892E	61FA
+0005	008930	B03C
+0006	0004F4	0000
+0007	0004F6	9530
+0008	00892A	4EFA

Figure 224. Incorrect Data

Your **first** assumption is that **incorrect** data is stored to this **memory location**. Assume this routine is in ROM since it is part of the operating system for your **circuit**. Since the ROM is programmed by **the software designer**, you have the software designer **verify** whether or not the data at address 8932 is correct. The software designer tells you that the data is **correct**. Now what do you do?

Now it's time to look at the **hardware** to see if it is causing **incorrect** data when the **microprocessor** reads this memory address. You decide you want to see what is happening on the address and data buses during this routine in the **time domain**.

In order to see the time domain, you need the **timing analyzer**.

What Additional Measurements Must I Make?

Since the problem exists during the routine that starts at address 8930, you decide you want to see the timing **waveforms** on the address and **data bus** when the routine is running. You also want to see the **control signals** that control the read cycle. You will then compare the waveforms with the **timing diagrams** in the 68000 data book.

Your **measurement**, then, requires verification of:

- **correct** timing of the control signals
- **stable** addresses and data during the memory read

The **control signals** you must check are:

- **system clock**
- **address strobe (AS)**
- **lower and upper data strobes (LDS and UDS)**
- **data transfer acknowledge (DTACK)**
- **read/write (R/W)**

How Do I Re-Configure the Logic Analyzer?

In order to **make** this measurement, you **must re-configure** the logic analyzer so Analyzer 2 is a timing analyzer. You leave Analyzer 1 as a state analyzer since you will use the state analyzer to trigger on address 8930.

Configure the logic analyzer so Analyzer 2 is a timing analyzer as shown:

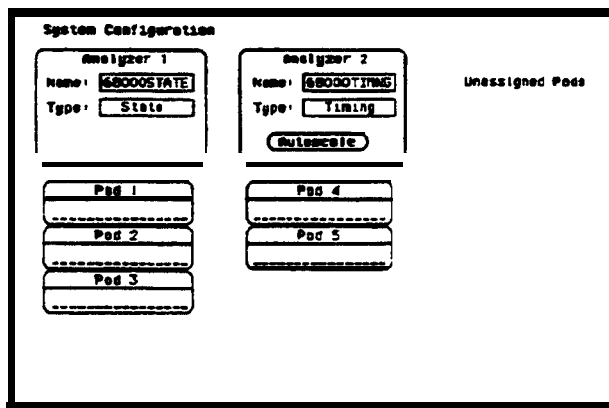


Figure 22-5. System Configuration Menu

Connecting the TimingAnalyzer Probes

At this point you would connect the probes of pods 4 and 5 as follows:

- Pod 4 bit 0 to address strobe (AS)
- Pod 4 bit 1 to the system clock
- Pod 4 bit 2 to low data strobe (LDS)
- Pod 4 bit 3 to upper data strobe (UDS)
- Pod 4 bit 4 to the read/write (R/W)
- Pod 4 bit 5 to data transfer acknowledge (DTACK)
- Pod 5 bits 0 through 7 to address lines A0 through A7
- Pod 5 bits 8 through 15 to data lines D0 through D7

Configuring the Timing Analyzer

Now that you have configured the system, you are ready to configure the timing analyzer. Configure the **TIMING FORMAT SPECIFICATION** menu as shown:

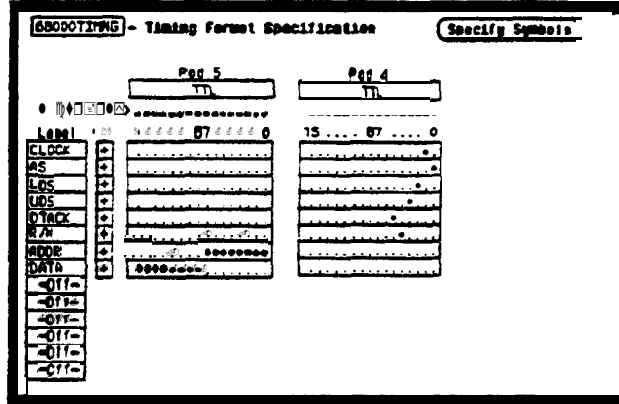


Figure 22-6. Timing Format Specification Menu

Configure the **TIMING TRACE SPECIFICATION** as shown:

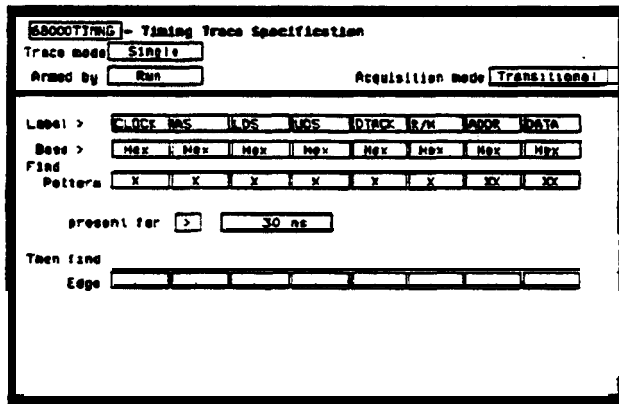


Figure 22-7. Timing Trace Specification Menu

Setting the Timing Analyzer Trigger

Your timing measurement requires the timing analyzer to display the timing waveforms present on the buses when the routine is running. Since you triggered the state analyzer on address 8930, you want to trigger the timing analyzer so the timing waveforms can be time correlated with the state listing.

To set up the logic analyzer so that the state analyzer triggers the timing analyzer, perform these steps:

1. Display the TIMING TRACE SPECIFICATION menu.
2. Place the cursor on the Armed by ___ field and press SELECT.
3. Place the cursor on the 68000STATE option in the pop-up and press SELECT.

Your timing trace specification should match the menu shown:

State Analyzer
Arms Timing
Analyzer

The screenshot shows the 'Timing Trace Specification' menu. The 'Armed by' field is set to '68000STATE'. The 'Acquisition mode' is 'Transitional'. The 'Label' row includes fields for CLOCK, MS, LDS, UDS, IOTACK, R/H, ADDR, and DATA. The 'Base' row has eight 'Hex' fields. The 'Find Pattern' row has eight 'X' fields. The 'present for' field is set to '30 ns'. The 'Then find Edge' row has eight empty fields.

Timing Trace Specification								
Trace mode	Single							
Armed by	68000STATE						Acquisition mode	Transitional
Label >	CLOCK	MS	LDS	UDS	IOTACK	R/H	ADDR	DATA
Base >	Hex	Hex	Hex	Hex	Hex	Hex	Hex	Hex
Find Pattern	X	X	X	X	X	X	XX	XX
present for >	30 ns							
Then find Edge								

Figure 22-8. Armed by 68000 STATE

Time Correlating the Data

In order to time correlate the data, the logic analyzer must store the timing relationships between states. Since the timing analyzer samples asynchronously and the state analyzer samples synchronously, the logic analyzer must use the stored timing relationship of the data to reconstruct a time correlated display.

To set up the logic analyzer to keep track of these timing relationships, turn on a counter in the STATE TRACE SPECIFICATION menu. The following steps show you how:

1. Display the STATE TRACE SPECIFICATION menu.
2. Place the cursor in the field just below Count on the right side of the display and press SELECT.
3. Place the cursor on the Time option and press SELECT. The counter will now be able to keep track of time for the time correlation.

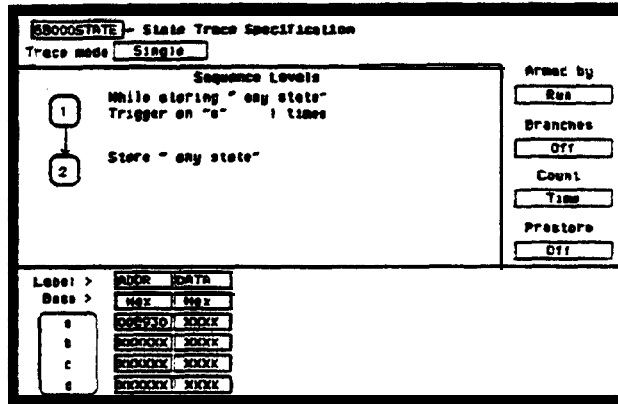


Figure 22-S. Count Set to Time

Re-Acquiring the Data

After you connect the probes of pods 4 and 5 to your circuit, all you have to do is press RUN. When the logic analyzer acquires the data it switches the display to the STATE LISTING menu unless you switched one of the other menus to the timing analyzer after reconfiguring the STATE TRACE menu. Regardless of which menu is displayed, change the display to the Mixed mode.

Mixed Mode Display

The Mixed mode display shows you both the STATE LISTING and TIMING WAVEFORMS menus simultaneously. To change the display to the Mixed mode:

1. Place the cursor on the field in the upper left corner of the display and press SELECT.
2. Place the cursor on Mixed mode and press SELECT. You will now see the mixed display as shown:

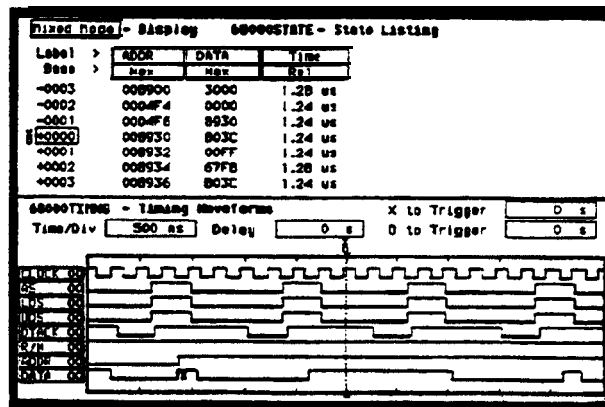


Figure 22-10. Mixed Mode Display

Interpreting the Display

In the Mixed mode display the state listing is in the top half of the screen and the timing waveforms are in the lower half. The important thing to remember is that you time correlated this display so you could see what is happening in the time domain during the faulty routine.

Notice that the trigger point in both parts of the display is the same as it was when the displays were separate. The trigger in the state listing is in the box containing + 0000 and the trigger of the timing waveform is the vertical dotted line.

As you look at the mixed display, you notice nothing wrong except the data at address 8932 is incorrect. However, you are seeing only one bit each of the address and the data. To see all the data and addresses in the timing waveform part of the display, you must overlap them.

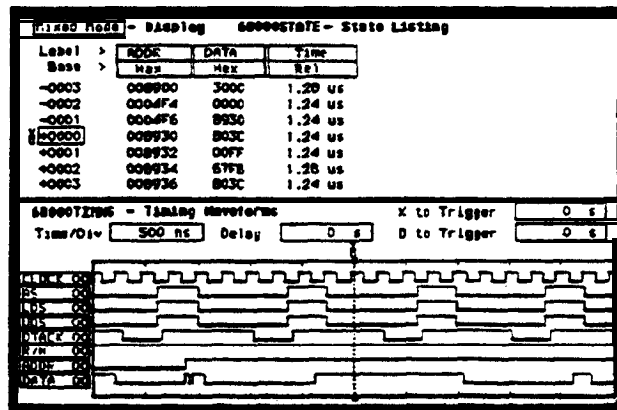


Figure 22-1 1. Interpreting the Display

Overlapping Timing Waveforms

Since you see **nothing** wrong with the timing waveforms so far, you **think unstable data may be on the data lines during the read cycle**. In order to see unstable data, you must be able to see all the data lines during the read and look for transitions. **Overlapping the waveforms** allows you to do this. To overlap waveforms, **follow these steps**

1. Place the cursor on the 00 of the ADDR 00 label and press SELECT. The following pop-up opens in which you specify the bit or bits of the address bus you want to overlap.
2. Rotate the KNOB until all is displayed and press SELECT. All the address bits will be overlapped on one line.
3. Repeat step 2 except overlap the data bits.

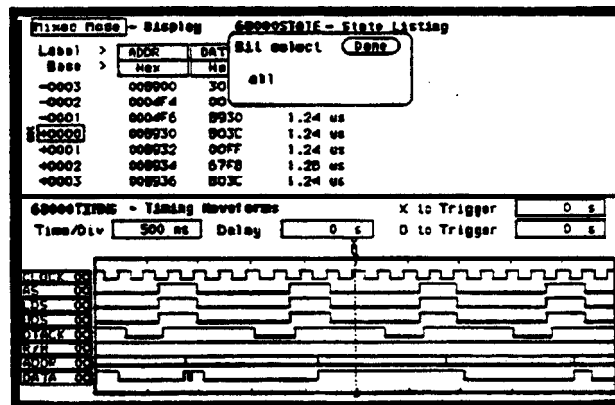


Figure 22-12 Overlapping Timing Waveforms

Finding the Answer

As you look at the overlapping waveforms, you notice there are transitions on the data lines during the read cycle, indicating the data is unstable. You have found the probable cause of the problem in this routine. Additional troubleshooting of the hardware will identify the actual cause.

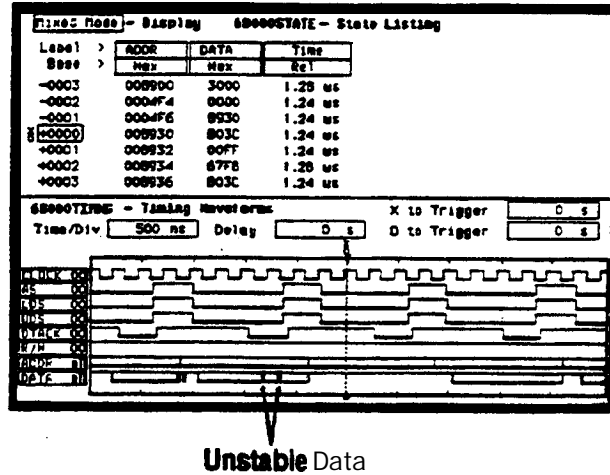


Figure 22-13. Unstable Data

Summary

You have just learned how to use the timing and state analyzers interactively to **find** a problem that first appeared to be a software problem, but actually was a **hardware** problem.

You have learned to:

- **trigger one analyzer with the other**
- **time correlate measurement data**
- interpret the Mixed mode display
- overlap **timing waveforms**

If you have an **HP 1651B**, you do not have **enough channels** to **simultaneously** capture all the data for a 68000. But, since you probably aren't working with **16-bit microprocessors**, **this exercise is still valuable because it shows you how to make the same kind of measurement on an eight-bit microprocessor.**

Error Messages

Introduction

This appendix lists the error messages that require corrective action to restore proper operation of the logic analyzer. There are several messages that you will see that are merely advisories and are not listed here. For example, "Load operation complete" is one of these advisories.

The message are listed in alphabetical order and in bold type.

Acquisition aborted. This message is displayed whenever data acquisition is stopped.

At least one edge is required. A state clock specification requires at least one clock edge. This message only occurs if you turn off all edges in the state clock specification.

Autoload file not of proper type. This message is displayed if any file other than an HP 1650B/51B configuration file is specified for an autoload file and the logic analyzer is powered up.

Autoscale aborted. This message is displayed when the STOP key is pressed or if a signal is not found 15 seconds after the initiation of autoscale.

BNC is being used as an ARM IN and cannot be used as an ARM OUT. This message is displayed when BNC arms machine 1 (or 2), machine 1 (or 2) arms machine 2 (or 1), and the BNC is specified as ARM OUT. It will not occur if BNC arms machine 1 (or 2), and machine 1 (or 2) arms BNC

Configuration not loaded. Indicates a bad configuration file. Try to reload the file again. If the configuration file will still not load, a new disk and/or configuration file is required.

Copy operation complete. Indicates the copy operation has either successfully completed or has been stopped.

Correlation counter overflow. The correlation counter overflows when the time from when one machine's trigger to the second machine's trigger exceeds the maximum count. It may be possible to add a "dummy" state to the second machine's trigger specification that is closer in time to the trigger of the first machine.

Data can not be correlated-Time count need to be turned on. "Count" must be set to "Time" in both machines to properly correlate the data.

Destination write protected-file not copied. Make sure you are trying to copy to the correct disk. If so, set the write protect tab to the non-protect position and repeat the copy operation.

File not copied to disk-check disk. The HP 1650B/51B does not support track sparing. If a bad track is found, the disk is considered bad. If the disk has been formatted elsewhere with track sparing, the HP 1650B/51B will only read up to the first spared disk.

Hardware ERROR: trace point in count block. Indicates the data from the last acquisition is not reliable and may have been caused by a hardware problem. Repeat the data acquisition to verify the condition. If this message re-appears, the logic analyzer requires the attention of service personnel.

Insufficient memory to load IAL - load aborted This message indicates that there is not a block of free memory large enough for the inverse assembler you are attempting to load even though there may be enough memory in several smaller blocks Try to load the inverse assembler again. If this load is unsuccessful, load the configuration and inverse assembler separately.

Invalid file name. Check the file name. A file name must start with an alpha character and cannot contain spaces or slashes (/).

Inverse assembler not loaded-bad object code. Indicates a bad inverse assembler file on the disk. A new disk or file is required.

Maximum of 32 channels per label. Indicates an attempt to assign more than 32 channels to a label. Reassign channels so that no more than 32 are assigned to a label.

No room **on destination-file** not **copied**. Indicates the **destination** disk doesn't have **enough** room for the **file** you are **attempting** to copy. Try **packing** the disk and **repeating** the copy operation. If this is **unsuccessful**, you will need to use a **different** disk.

(x) Occurrences Remaining in Sequence. Indicates the logic analyzer is waiting for **(x)** number of occurrences in a sequence level of the trigger specification before it can go on to the next sequence level.

PRINT has been stopped. This message appears when the print operation has been stopped.

(x) Secs Remaining in Trace. Indicates the amount of time **remaining** until acquisition is complete in **Glitch** mode.

Search failed - O pattern not found. Indicates the **O** pattern does not exist in the acquired data. Check for a correct **O** marker pattern specification.

Search failed - X pattern not found. Indicates the **X** pattern does not exist in the acquired data. Check for a correct **X** marker pattern specification.

Slow Clock or **Waiting for Arm**. Indicates the state analyzer is waiting for a clock or arm from the other machine. Re-check the state clock or arming specification.

Slow or missing Clock. Indicates the state analyzer has not **recognized** a clock for 100 ms. Check for a **missing** clock if the intended clock is faster than 100 ms. If clock is present but is slower than 100 ms, the data will still be acquired when a clock is recognized and should be valid.

Specified inverse assembler not found. Indicates the inverse assembler specified cannot be found on the disk.

State **clock violates overdrive specification**. Indicates the data from the last acquisition is not reliable due to the state **clock** signal not **being** reliable. Check the **clock** threshold for proper setting and the probes for proper grounding.

States **Remaining** to Post **Store**. Indicates the number of states required until memory is **filled** and acquisition is **complete**.

Time count need to be turned on. This message appears when the logic analyzer attempts to time correlate data and "Count" is not set to "Time."

Transitions Remaining to Post Store. Indicates the number of transitions required until memory is filled and acquisition is complete.

Unsupported destination **format-file** not copied- Indicate5 the disk you have attempted to copy to is either not formatted or formatted in a **format not used by the logic analyzer.** Format the disk or use a properly formatted disk and repeat the copy operation.

Value out of range. Set to **limit.** Indicates an attempt to enter a value that is out of range for the specific variable. The logic analyzer will set the value to the limit of the variable range automatically.

waiting for Arm. Indicates the arming condition has not occurred.

Waiting for Prestore. Indicates the prestore condition has not occurred (timing analyzer only).

Waiting for Trigger. Indicates the trigger condition has not occurred.

Warning: Chips not successfully running. Indicates the acquisition chips in the logic analyzer are not running properly. Press STOP and then RUN again. If the warning message reappears, refer the logic analyzer to service personnel.

Warning: Chips not successfully stopped. indicates the acquisition chips in the logic analyzer are not stopping properly. Press RUN and then STOP again. If the warning message reappears, refer the logic analyzer to service personnel.

Warning: Duplicate label name. Indicates an attempt to assign an existing name to a new label.

Warning: Daplii symbol name. Indicates an attempt to assign an existing name to a new symbol.

Warning: Invalid file type. Indicates an attempt to load an invalid file type. For example, the SYSTEM file can only be loaded on power-up and if you attempt to load it from the I/O menu, this message will appear.

Warning: No clock edge in other clock, added clock edge. This message only occurs in a state analyzer using mixed or demultiplexed clocks. It indicates there is no edge specified in either the master or slave clock. There must be at least one edge in each of the clocks.

Warning: Symbol memory full. Max 200 symbols. Indicates an attempt to store more than 200 symbols.

Warning: Run HALTED due to variable change. Indicates a variable has been changed during data acquisition in the continuous trace mode. The data acquisition will be halted and this message will be displayed when any variable affecting the system configuration, clock thresholds, dock multiplexing, or trace specification menus is changed during data acquisition.

Installation and Maintenance

Introduction

This appendix contains information and instructions necessary for preparing the HP 1650B/51B Logic Analyzers for use. Included in this section are inspection procedures, power requirements packaging information, and operating environment. It also tells you how to load the operating system and turn the logic analyzer on. Maintenance that you can do as an operator is included in this appendix.

Initial Inspection

Inspect the shipping container for damage. If the shipping container or cushioning material is damaged, it should be kept until the contents of the shipment have been checked for completeness and the instrument has been checked mechanically and electrically. Accessories supplied with the instrument are listed under Accessories Supplied in section 1 of this manual. An overview of the self-test procedure is in Appendix C of this manual. The complete details of the procedure are in Chapter 6 of the *Service Manual*. Electrical performance verification functions are also in Chapter 3 of the *Service Manual*.

If the contents are **incomplete**, if there is mechanical damage or defect, or if the instrument does not pass the **Self Test Performance Verification**, notify the **nearest Hewlett-Packard Office**. **If the shipping container is damaged, or the cushioning materials show signs of stress, notify the carrier as well as the Hewlett-Packard Office. Keep all shipping materials for the carrier's inspection.** The Hewlett-Packard office will arrange for repair or replacement at HP option without waiting for claim settlement.

Operating Environment

You may operate your logic analyzer in a normal lab or office type environment without any additional considerations. If you intend to use it in another type of environment, refer to Table D-2 in Appendix E for complete operating environment specifications. Note the non-condensing humidity limitation. Condensation within the instrument cabinet can cause poor operation or malfunction. Protection should be provided against temperature extremes which cause condensation.

Ventilation

You must provide an unrestricted airflow for the fan and ventilation openings in the rear of the logic analyzer. However, you may stack the logic analyzer under, over, or in-between other instruments as long the surfaces of the other instruments are not needed for their ventilation.

Storage and Shipping

This instrument may be stored or shipped in environments within the following limitations:

- Temperature: -40°C to $+75^{\circ}\text{C}$
- Humidity: Up to 90% at 65°C
- Altitude: Up to 15,300 meters (50,000 feet)

Tagging for Service

If the instrument is to be shipped to a Hewlett-Packard office for service or repair, attach a tag to the instrument identifying owner address of owner, complete instrument model and serial numbers and a description of the service required.

Original Packaging

If the original packaging material is unavailable or unserviceable materials identical to those used in factory packaging are available through Hewlett-Packard offices. If the instrument is to be shipped to a Hewlett-Packard office for service, tag the instrument (see "Tagging for Service" in this appendix). Mark the container FRAGILE to ensure careful handling. In any correspondence, refer to the instrument by model number and full serial number.

Other Packaging The following general **instructions** should be followed for repacking with **commercially** available materials.

1. **Wrap the instrument in heavy paper or plastic.**
2. Use a **strong shipping container**. A double-wall carton made of 350 lb. test material is adequate.
3. Use a **layer of shock-absorbing material 70 to 100 mm (3 to 4 inches)** thick around **all sides** of the instrument to **firmly cushion** and prevent movement inside the container. Protect the control **panel with cardboard**.
4. seal the shipping **container securely**.
5. **Mark the shipping container FRAGILE** to ensure careful handling.
6. In any **correspondence**, refer to the instrument by **model** number and **full** serial number.

Power Requirements

The HP 1650B/51B requires a **power source** of either 115 or 230 Vac **-22% to + 10%**; single phase, 48 to 66 Hz; 200 Watts **maximum power**.

Power Cable

This instrument is provided with a three-wire power cable. When connected to an appropriate AC power outlet, this cable grounds the instrument cabinet. The type of power cable plug shipped with the instrument depends on the country of destination. Refer to Table B-1 for power plugs and HP part numbers for the available plug











- -

Warning



BEFORE CONNECTING THIS INSTRUMENT, the protective earth terminal of the instrument must be connected to the protective conductor of the (Mains) power cord. The Mains plug must be inserted in a socket outlet provided with a protective earth contact. The protective action must not be negated by the use of an extension cord (power cable) without a protective conductor (grounding). Grounding one conductor of a two conductor outlet does not provide an instrument ground.

Table B-I. Power Cord Configurations

PLUG TYPE	CABLE PART NO.	PLUG DESCRIPTION	LENGTH IN/CM	COLOR	COUNTRY
OPT 900  250V	8120-1351 8120-1703	Straight +BS1363A 90°	30/228 90/228	Gray Mint Gray	United Kingdom, Cyprus, Nigeria, Zimbabwe, Singapore
OPT 901  250V	8120-1289 8120-0998	Straight +NZS186/ASC 90°	78/200 87/221	Gray Mint Gray	Australia New Zealand
OPT 902  250V	8120-1689 8120-1692 8120-2657	Straight +CEE7-V11 90° Straight (Shielded)	78/200 79/200 79/200	Mint Gray Mint Gray Coco Brown	East and West Europe, South Arabia, S. Africa, India (Unauthorized in many nations)
OPT 903**  125V	8120-1378 8120-1521 8120-1982	Straight +NEMA-15P 90° Straight (Medical) UL544	30/228 30/228 36/244	Jade Gray Jade Gray Black	United States, Canada, Mexico, Philippines, Israel
OPT 904**  250V	8120-0998	Straight +NEMA-15P	30/228	Black	United States, Canada
OPT 905  250V	8120-1298 8120-1625	CEE22-V1 (System Cabinet Use) 250V	20/78 36/244	Jade Gray	For interconnecting system components and peripherals. United States and Canada only
OPT 906  250V	8120-2104 8120-2296	Straight +CEV1011 1959-24507 Type 1Z 90°	78/200 79/200	Mint Gray Mint Gray	Switzerland
OPT 912  250V	8120-2936 8120-2937	Straight +ENCK107 90°	78/200 79/200	Mint Gray Mint Gray	Denmark
OPT 917  250V	8120-4211 8120-4600	Straight SABS164 90°	78/200 79/200	Jade Gray	Republic of South Africa India
OPT 918  100V	8120-4733 8120-4734	Straight 811: 90°	90/230 90/230	Dark Gray	Japan

*Part number shown for plug is industry identifier for plug only. Number shown for cable is HP part number for complete cable including plug.
 **These cords are included in the CSA certification approval of the equipment.
 E=Earth Ground
 L=Line
 N=Neutral

Removing Yellow Shipping Disk

Your logic analyzer is shipped with a protective yellow shipping disk in the disk drive. Before you can insert the operating system disk you must remove the yellow shipping disk. Press the disk eject button as shown in figure B-1. The yellow shipping disk will pop out part way so you can pull it out of the disk drive.

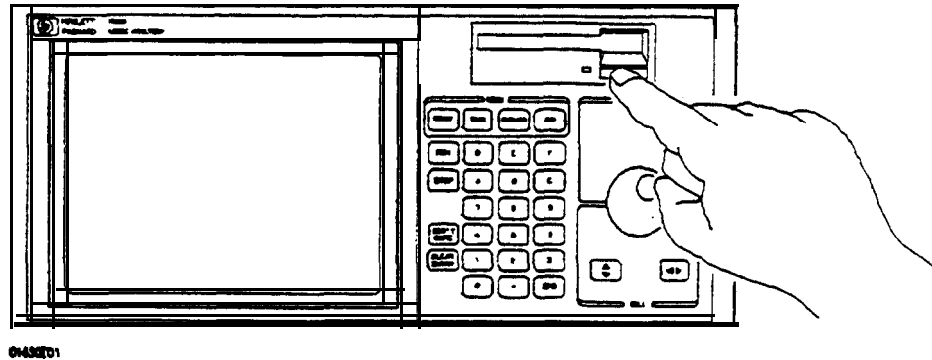


Figure E1. Removing **Yellow Shipping Disk**

Selecting the Line Voltage

The line voltage selector has been factory set to the line voltage used in your country. It is a good idea to check the setting of the line voltage selector so you become familiar with what it looks like. If the setting needs to be changed, follow the procedure in the next paragraph.

Caution



You can damage the logic analyzer if the module is not set to the correct position.

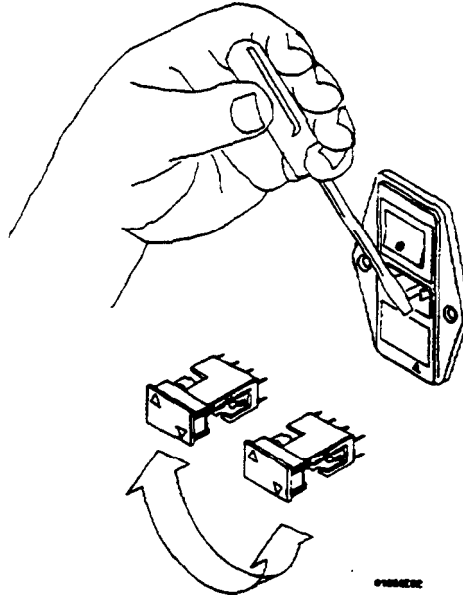


Figure B-2 Selecting the Line Voltage

You change the proper line voltage by **pulling the fuse module out and reinserting it with the proper arrows aligned**. To remove the fuse module, carefully pry at the top center of the module (as shown) until you can grasp and pull it out by hand.

Checking for the Correct Fuse

If you find it necessary to check or change fuses, remove the fuse module and look at **each** fuse for its **amperage** and voltage. Refer to **figure B-3** to locate the **115 V** and **230 V** fuse locations. To remove the fuse module, carefully pry at the top **center** of the module (see **figure B-2**) until you can **grasp and pull it out by hand**.

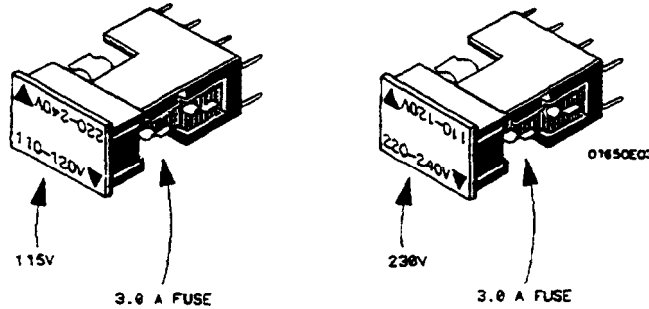


Figure B-3. Checking for the Correct Fuse

Applying Power

When power is applied to the **HP 1650B/51B**, a power-up self test will be performed **automatically**. For information on the power-up self test, refer to **Appendix C** and **Section 3** of the *Service Manual*.

Loading the Operating System

Before you can operate the instrument, you must load the operating system from the operating system disk. You received two identical operating system disks. You should mark one of them **Master** and store it in a safe place. Mark the other one **Work** and use only the work copy. This will provide you with a back-up in case your work copy becomes corrupt.

Caution



To prevent damage to your operating system disk, **DO NOT** remove the disk from the disk drive while it is running. Only remove it after the indicator light has gone out.

Installing the Operating System Disk

To load the logic analyzer's operating system, you must install the disk as shown below before you turn on the power. When the disk snaps into place, the disk eject button pops out and you are ready to turn on the logic analyzer.

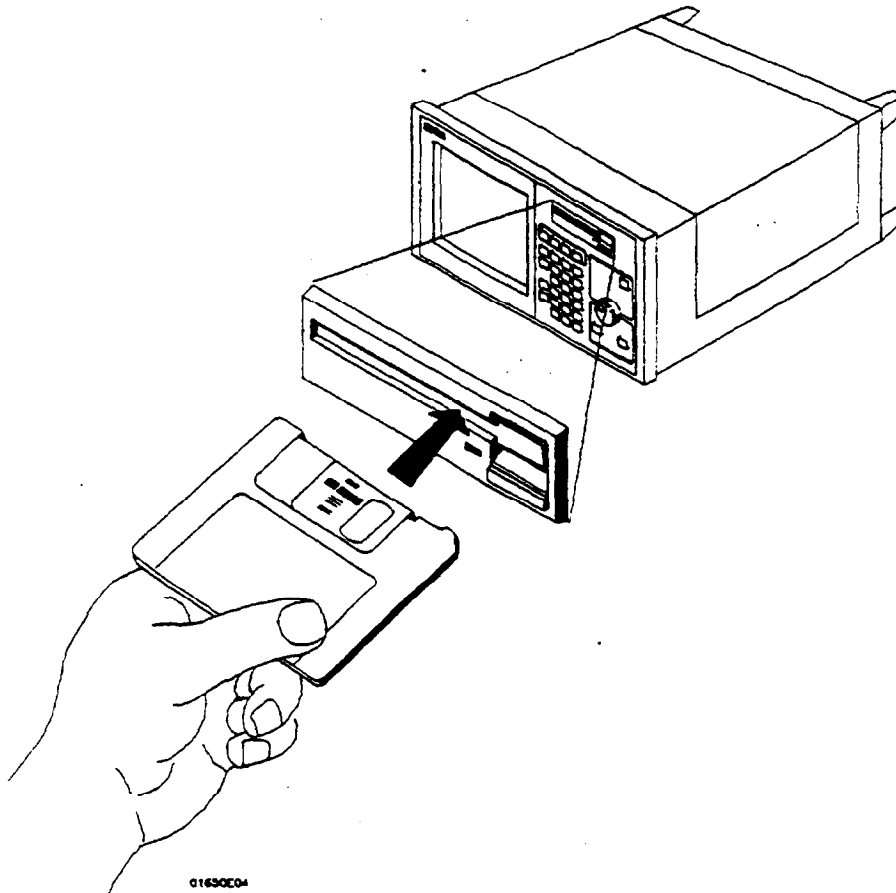


Figure B-4. Installing the Operating System **Disk**

The logic analyzer will read the disk and load the operating system. It will also run self-tests before it is ready for you to operate.

Line Switch

The line switch is located on the rear panel. You turn the instrument on by pressing the 1 on the rocker switch. Make sure the operating system disk is in the disk drive before you turn on the logic analyzer. If you forget the disk, don't worry, you won't harm anything. You will merely have to repeat the turn-on procedure with the disk in the drive.

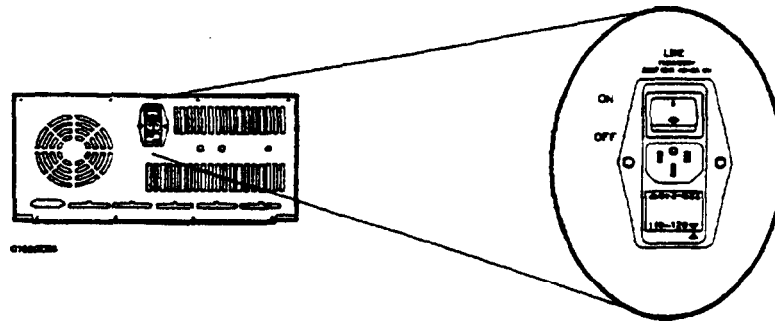


Figure s-5. Line switch

Intensity Control

Once you have turned the instrument on, you may want to set the display intensity to a level that's more comfortable for you. You do this by turning the INTENSITY control on the rear panel.

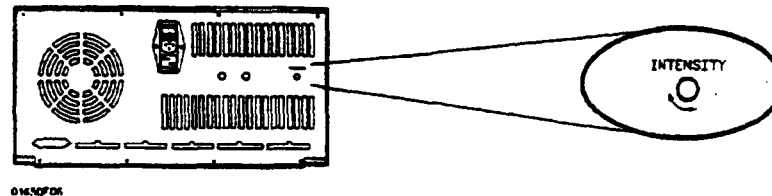


Figure B-6. Intensity Control

Power-Up Self-Test

When you turn on the logic analyzer, it performs a series of self-tests. When it has successfully completed these tests, it loads the operating system into memory from the disk

When the logic analyzer has completely loaded the operating system it displays the System Configuration menu as shown below.

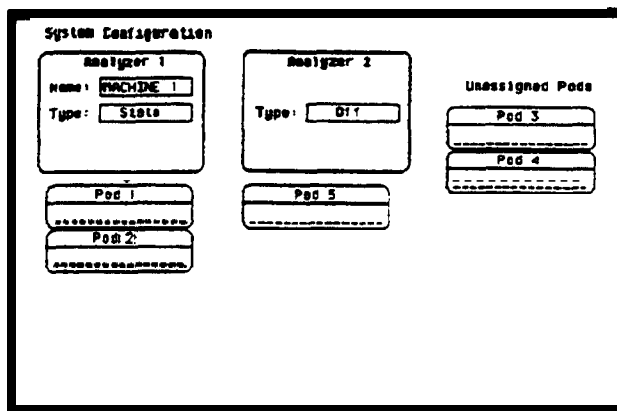


Figure B-7. System Configuration Menu

Note 

This is the HP 1650B System Format Specification menu. If you have an HP 1651B, pod 1 will be assigned to analyzer 1 and pod 2 will be assigned to analyzer 2. There won't be any pods in the Unassigned Pods area of the display.

Operator's Maintenance

The only maintenance you need to do is clean the instrument exterior and periodically check the rear panel for air restrictions.

Use only MILD SOAP and WATER to clean the cabinet and front panel. DO NOT use a harsh soap which will damage the water-base paint finish of the instrument,

Operator Self-Tests

Introduction

This appendix gives you an overview of the self tests the logic analyzer runs when you turn it on. You can also access the self tests from the I/O menu. This appendix is not intended to provide service information, but to acquaint you with the tests. If service is required, it should be performed by qualified service personnel.

Self -Tests

The power-up self test is a set of tests that are automatically performed when you apply power to the logic analyzer. You may perform the self tests individually to have a higher level of confidence that the instrument is operating properly. A message that the instrument has failed a test will appear if any problem is encountered during a test. The individual self tests are listed in the self test menu which is accessed via the I/O menu. The HP 1650B/51B self tests are on the operating system disk and the disk is required to run the tests.

Power-Up Self-Test

The power-up self test is automatically initiated at power-up by the HP 1650B/51B Logic Analyzer. The revision number of the operating system firmware is given in the upper right of the screen during the power-up self test. As each test is completed, either "passed" or "failed" will be displayed before the name of the test as shown.

PERFORMING POWER-UP SELF TESTS

passed ROM test
 passed RAM test
 passed Interrupt test
 passed Display test
 passed Keyboard test
 passed Acquisition test
 passed Threshold test
 passed Disk test

LOADING SYSTEM FILE

As indicated by the last message, the HP 1650B/51B will automatically load the operating system from the disk in the disk drive. If the operating system disk is not in the disk drive, the message "SYSTEM DISK NOT FOUND" will be displayed at the bottom of the screen and "NO DISK" will be displayed in front of disk test in place of "passed."

If the "NO DISK" message appears, insert the operating system disk into the disk drive, and press any front-panel key.

Selectable Self Tests

Seven self tests may be accessed individually in the Self

Test menu. The seven selectable self tests are:

- Acquisition
- RS-232C
- External Trigger BNCs .
- Keyboard
- RAM
- R O M
- Disk Drive
- Cycle through all tests

To select a test, place the cursor on the test name and press SELECT. A pop-up menu appears with a description of the test. The self test does not begin until the cursor is placed on Execute and the SELECT key is pressed.

When the test is complete, either "Passed", "Failed", or "Tested" will be displayed in the Self Test menu in front of the test. These tests are also used as troubleshooting aids. If a test fails, refer to Section 6 of the Service manual for information on the individual tests used for troubleshooting.

Specifications and Operating Characteristics

introduction

This appendix lists the specifications, operating characteristics, and supplemental characteristics of the HP 1650B and HP 1651B Logic Analyzers.

Specifications

Probes Minimum Swing: 600 mV peak-to-peak.

Threshold Accuracy:

Voltage	Range Accuracy
- 2.0 V to + 2.0 V	+ 150 mV
- 9.9 v to - 2.1 v	+ 300 mV
+ 2.1 V to + 9.9 V	- 300 mV

State Mode

Clock Repetition Rate: Single phase is 35 MHz maximum (25 MHz on the HP 1651B). With time or state counting, minimum time between states is 60 ns. Both mixed and demultiplexed clocking use master-slave clock timing; master clock must follow slave dock by at least 10 ns and precede the next slave clock by 50 ns.

Clock Pulse Width: ≥ 10 ns at threshold.

Setup Time: Data must be present prior to clock transition, ≥ 10 ns.

Hold **Time**: Data **must** be present after rising clock **transition**; **0 ns**.

Data must be present after **falling** clock transition, **0 ns (HP 1651B)**; **data must be present after falling L clock transition, 0 ns (HP 1650B)**; **data must be present after falling J, K, M, and N clock transition, 1 ns (HP 1650B)**.

Timing Mode

Minimum Detectable Glitch: **5 ns** wide at the threshold

Characteristics

Probes input **RC**: **100 k Ω \pm 2%** shunted by **approximately 8 pF** at the probe tip.

TTL Threshold Preset: **+ 1.6 volts**.

ECL Threshold Preset: **- 1.3 volts**.

Threshold Range: **- 9.9 to + 9.9 volts in 0.1 V increments**.

Threshold Setting: Threshold **levels may be defined** for pods 1 and 2 **individually (HP 1651B)**. Threshold levels may be defined for pods **1, 2, and 3 individually and one threshold may be defined for pods 4 and 5 (HP 1650B)**.

Minimum Input Overdrive: **250 mV or 30% of the input amplitude whichever is greater**.

Maximum Voltage: **\pm 40 volts peak**

Dynamic Range: **\pm 10 volts about the threshold**.

Measurement Configurations

Analyzer Configurations:

<u>Analyzer 1</u>	<u>Analyzer 2</u>
Timing	Off
Off	Timing
State	Off
Off	State
Timing	State
State	Timing
State	State
Off	Off

Channel Assignment: Each group of 16 channels (a pod) can be assigned to Analyzer 1, Analyzer 2, or remain unassigned. The HP 1650B contains 5 pods; the HP 1651B contains 2 pods.

State Analysis

Memory Data Acquisition: 1024 samples/channel.

Trace specification

Clocks: Five clocks (HP 1650B) or two clock (HP 1651B) are available and can be used by either one or two state analyzers at any time. Clock edges can be ORed together and operate in single phase, two phase demultiplexing, or two phase mixed mode. Clock edge is selectable as positive, negative, or both edges for each clock.

Clock Qualifier: The high or low level of four ORed clocks (HP 1650B) or one clock (HP1651B) can be ANDed with the clock specification. Setup time: 20 ns; hold time: 5 ns.

Pattern Recognizers: Each recognizer is the AND combination of bit (0, 1, or X) patterns in each label. Eight pattern recognizers are available when one state analyzer is on. Four are available to each analyzer when two state analyzers are on.

Range Recognizers: Recognizes data which is numerically between or on two specified patterns (ANDed combination of 0s and/or 1s). One range term is available and is assigned to the first state analyzer turned on. The maximum size is 32 bits.

Qualifier: A user-specified term that can be anystate., nostate, a single pattern recognizer, range recognizer, or logical combination of pattern and range recognizers.

Sequence Levels: There are eight levels available to determine the sequence of events required for trigger. The trigger term can occur anywhere in the first seven sequence levels.

Branching: Each sequence level has a branching qualifier. When satisfied, the analyzer will restart the sequence or branch to another sequence level.

Occurrence Counter: Sequence qualifier may be specified to occur up to 65535 times before advancing to the next level.

Storage Qualification: Each sequence level has a storage qualifier that specifies the states that are to be stored.

Enable/Disable: Defines a window of post-trigger storage. States stored in this window can be qualified.

Prestore: Stores two qualified states that precede states that are stored.

Tagging

State Tagging: Counts the number of qualified states between each stored state. Measurement can be shown relative to the previous state or relative to trigger. Maximum count is 4.4 X (10 to the 12th power).

Time Tagging Measures the time between stored states, relative to either the previous state or the trigger. Maximum time between states is 48 hours.

With tagging on, the acquisition memory is halved; minimum time between states is 60 ns.

Symbols **Pattern Symbols:** User can define a mnemonic for the specific bit pattern of a label. When data display is SYMBOL, mnemonic is displayed where the bit pattern occurs. Bit pattern can include 0s, 1s, and don't cares.

Range Symbols: User can define a mnemonic covering a range of values. Bit pattern for lower and upper limits must be defined as a pattern of 0s and 1s. When data display is SYMBOL, values within the specified range are displayed as mnemonic \pm offset from base of range.

Number of Pattern and Range Symbols: 200 total. Symbols can be down-loaded over RS-232C.

Timing Analysis

Transitional Timing Mode Sample is stored in acquisition memory only when the data changes. A time tag stored with each sample allows reconstruction of waveform display. Time covered by a full memory acquisition varies with the number of pattern changes in the data.

Sample Period: 10 ns.

Maximum Time Covered by Data: 5000 seconds.

Minimum Time Covered by Data: 10.24 μ s.

Glitch Capture Mode Data sample and glitch information stored every sample period.

Sample Period: 20 ns to 50 ms in a 1-2-5 sequence dependent on sec/div and delay settings.

Memory Depth: 512 samples/channel.

Time Covered by Data: Sample period x 512.

Waveform Display Sec/div: 10 ns to 100 s; 0.01% resolution.

Delay: – 2500 s to 2500 s; **presence** of data dependent on the number of transitions in data between trigger and trigger plus delay (transitional timing).

Accumulate: Waveform display is not erased between successive acquisitions.

Overlay Mode: Multiple channels can be displayed on one waveform display line. Primary use is to view summary of bus activity.

Maximum Number of Displayed Waveforms: 24

Channel-to-Channel Skew: 4 ns typical.

Time Interval Accuracy: \pm (sample period + channel-to-channel skew + 0.01% of time interval reading).

Trigger Specification

Asynchronous Pattern: Trigger on an asynchronous pattern less than or greater than specified duration. Pattern is the logical AND of specified low, high, or don't care for each assigned channel. If pattern is valid but duration is invalid, there is a 20 ns reset time before looking for patterns again.

Greater Than Duration: Minimum duration is 30 ns to 10 ms with 10 ns or 0.01% resolution, whichever is greater. Accuracy is + 0 ns to – 20 ns. Trigger occurs at pattern + duration.

Less Than Duration: Maximum duration is 40 ns to 10 ms with 10 ns or 0.01% resolution, whichever is greater. Pattern must be valid for at least 20 ns. Accuracy is + 20 ns to – 0 ns. Trigger occurs at the end of the pattern.

Glitch/Edge Triggering: Trigger on glitch or edge following valid duration of asynchronous pattern while the pattern is still present. Edge can be specified as rising, falling or either. Less than duration forces glitch and edge triggering off.

Measurement and Display Functions

Autoscale (Timing Analyzer Only)

Autoscale searches for and displays channels with activity on the pods assigned to the timing analyzer.

Acquisition Specifications

Arming: Each analyzer can be armed by the run key, the other analyzer, or the external trigger in port.

Trace Mode: Single mode acquires data once per trace specification; repetitive mode repeats single mode acquisitions until stop is pressed or until time interval between two specified patterns is less than or greater than a specified value, or within or not within a specified range. There is only one trace mode when two analyzers are on.

Labels

Channels may be grouped together and given a six character name. Up to 20 labels in each analyzer may be assigned with up to 32 channels per label. Primary use is for naming groups of channels such as address, data, and control busses.

Indicators

Activity Indicators: Provided in the Configuration, State Format and Timing Format menus for identifying high, low, or changing states on the inputs.

Markers: Two markers (X and 0) are shown as dashed lines on the Timing Waveforms display.

Trigger: Displayed as a vertical dashed line in the timing waveform display and as line 0 in the state listing display.

Marker Functions **Time Interval:** The X and 0 markers **measure the time interval between one point on a timing waveform and trigger, two points on the same timing waveform, two points on different waveforms, or two states (time tagging on).**

Delta States (State Analyzer Only): The X and 0 markers **measure the number of tagged states between one state and trigger, or between two states.**

Patterns: The X and 0 markers **can be used to locate the nth occurrence of a specified pattern before or after trigger, or after the beginning of data. The 0 marker can also find the nth occurrence of a pattern before or after the X marker.**

Statistics: X to 0 **marker statistics are calculated for repetitive acquisitions. Patterns must be specified, for both markers and statistics are kept only when both patterns can be found in an acquisition. Statistics are minimum X to 0 time, maximum X to 0 time, average X to 0 time, and ratio of valid runs to total runs.**

Run/Stop Functions **Run:** Starts acquisition **of data in specified trace mode.**

Stop: In single trace mode or the **first run** of a repetitive **acquisition, STOP halts acquisition and displays the current acquisition data.** For subsequent runs in repetitive mode, **STOP halts acquisition of data and does not change current display.**

Data Display/Entry **Display Modes:** state listing state waveform; state chart; state compare; timing waveforms; interleaved, time-correlating listing of two state analyzers (time tagging on); time-correlated state listing and timing waveform display (state listing in upper half, timing waveform in lower half, and time tagging on).

Timing Waveform: Pattern readout of timing waveforms at X or 0 marker.

Bases: Binary, Octal, Decimal, Hexadecimal, ASCII (display only) and User-defined symbols.

State Compare Mode

Performs **post-processing** bit-by-bit **comparison** of the acquired state **data and compare data image**.

Compare Image. Created **by** copying a state **acquisition** into **the compare image buffer**. Allows **editing of any bit in the compare image to a 1, 0, or don't care**.

Compare Image Boundaries. Each **channel (column) in the compare image can be enabled or disabled via bit masks in the compare image**. Upper and lower ranges of states (rows) **in the compare image can be specified**. **Any data bits that do not fall within the enabled channels and the specified range are not compared**.

Stop Measurement. **Repetitive acquisitions may be halted when the comparison between the current state acquisition and the current compare image is equal or not equal**.

Displays. Compare Listing display shows **the compare image and bit masks**. **Difference Listing display highlights differences between the current state acquisition and the current compare image**.

State X-Y Chart Display

Plots **value of specified label** (cm y-axis) vs. states or another label (on **x-axis**). **Both axes can be scaled by the user**.

Markers. correlated to state **listing**, state **compare**, and state **waveform displays**. Available as **pattern, time or statistics (with time counting on)**, and states (with state **counting on**).

Accumulate. **Chart display is not erased between successive acquisitions**.

State Waveform Display

Displays **state acquisition in waveform format**.

States/div. 1 to 104.

Delay. 0 to 1024.

Accumulate. Waveform display **is** not erased between **successive acquisitions**.

Overlay Mode. Multiple channels can be displayed on one waveform **display line**. Primary use is to view summary of bus activity.

Maximum **Number of Displayed** Waveforms. 24.

Markers. Correlated to state listing, state compare, and state chart displays. **Available** as pattern, time or statistics (with time **counting** on), and states (**with state counting** on).

Operating Environment

Temperature: Instruments, 0° to 55° C (+ 32° to 131° F); probes and cables, 0° to 65° C (+ 32° to 149° F). **Recommended** temperature range for disk media, 10° to 50° C (+ 50° to 122° F).

Humidity: Instruments **up** to 95% relative humidity at + 40° C; (104° F). **Recommended** humidity range for disk media, 8% to 80% relative humidity at + 40° C (+ 104° F).

Altitude: To 4600 m (15,000 ft).

Vibration

Operating: Random vibration 5-500 Hz, 10 minutes per axis, \approx 241 g (rms).

Non-operating: Random vibration 5-500 Hz, 10 minutes per axis, \approx 2.41 g (rms); and swept sine resonant search, 5-500 Hz, 0.75 g (O-peak), 5 minute resonant dwell @ 4 resonances per axis.


Weight: 10.0 kg (22 lbs) net; 18.2 kg (40 lbs) shipping.

Power: 115V/230V, 48-66 Hz, 200 W _{max}.

Dimensions

Notes: 1. Dimensions are for general information **only**. If **dimensions are required for building special enclosures, contact your HP field engineer.**

2. **Dimensions** are in **millimeters** and (inches).

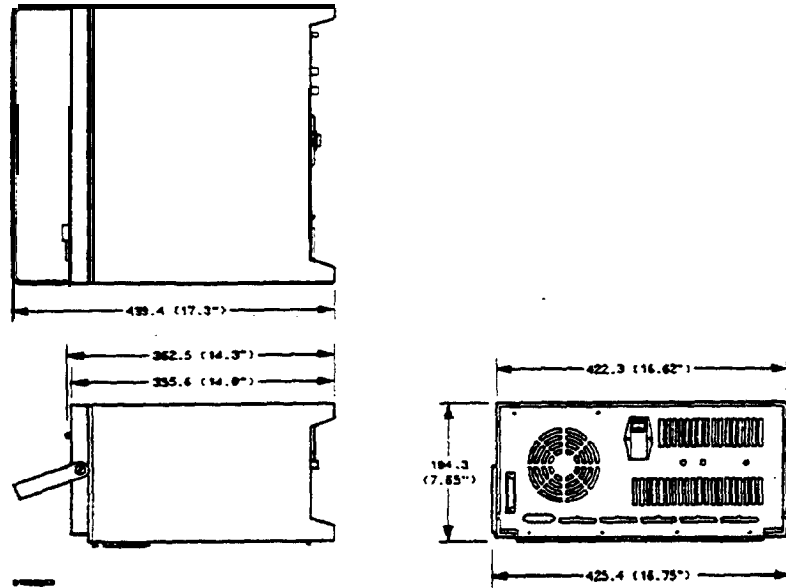

HP 1650B/HP 1651B
Front-Panel Reference

Specifications and Operating Characteristics
D-11

Microprocessor Specific Measurements

Introduction

This appendix contains information about the optional accessories available for microprocessor specific measurements. In-depth measurement descriptions are included in the operating notes that come with each of these accessories. The accessories you will be introduced to in this appendix are the preprocessor modules and the HP 10269C General Purpose Probe Interface.

Microprocessor Measurements

A preprocessor module enables you to quickly and easily connect the logic analyzer to your microprocessor under test. Most of the preprocessor modules require the HP 10269C General Purpose Probe Interface. The preprocessor descriptions in the following sections indicate which preprocessors require it.

Included with each preprocessor module is a 3.5-inch disk which contains a configuration file and an inverse assembler file. When you load the configuration file, it configures the logic analyzer for making state measurements on the microprocessor for which the preprocessor is designed. It also loads in the inverse assembler file.

The inverse assembler file is a software routine that will display captured information in a specific microprocessor's mnemonics. The DATA field in the STATE LISTING is replaced with an inverse assembly field (see Figure E-1). The inverse assembler software is designed to provide a display that closely resembles the original assembly language listing of the microprocessor's software. It also identifies the microprocessor bus cycles captured, such as Memory Read, Interrupt Acknowledge, or I/O write.

0000STATE - State Listing		Invert	Time X to Trigger	0 s
Markers		Time	Time 0 to Trigger	0 s
			Time X to 0	0 s
Label >	ADDR	HEX000 Mnemonic	Time	STAT
Base >	Hex	Hex	Rel	Hex
-0002	0004F4	ORI.B #30.D0		28
-0001	0004F5	BSO program read	1.24 us	28
+0000	000930	CHP.B #FF.D0	1.28 us	30
+0001	000932	GOFF program read	1.24 us	30
+0002	000934	RES.B 00092E	1.24 us	30
+0003	000936	CHP.B #..D0	1.24 us	30
+0004	00092E	BSR.B 00092A	1.76 us	30
+0005	000930	BSO unused prefetch	1.24 us	30
+0006	0004F4	BSO program write	2.00 us	29
+0007	0004F5	BSO program write	1.48 us	29
+0008	00092A	JMP 000925(PC1)	1.28 us	30
+0009	00092C	FFSA program read	1.24 us	30
+0010	00092E	BSR.B 00092E	1.72 us	30
+0011	00092E	BSO unused prefetch	1.28 us	30

Figure E-1. State Listing with Mnemonics,

Microprocessors Supported by Preprocessors

This section lists the microprocessors that are supported by Hewlett-Packard preprocessors and the logic analyzer model that each preprocessor requires. Most of the preprocessors require the HP 10269C General Purpose Probe Interface. The HP 10269C accepts the specific preprocessor PC board and connects it to five connectors on the general purpose interface to which the logic analyzer probe cables connect.

Note



This appendix lists the preprocessors available at the time of printing. However, new preprocessors may become available as new microprocessors are introduced. Check with the nearest Hewlett-Packard sales office periodically for availability of new preprocessors.

Z80 CPU Package: 40-pin DIP

Accessories Required: HP 10300B Preprocessor
HP 10269C General Purpose Probe Interface

Maximum Clock Speed: 10 MHz clock input

Signal Line Loading: Maximum of one 74LS TTL load + 35 pF on any line

Microprocessor Cycles Identified: Memory read/write
I/O read/write
Opcode fetch
Interrupt acknowledge
RAM refresh cycles

Maximum Power Required: 0.3A at + 5 V dc, supplied by logic analyzer

Logic Analyzer Required: HP 1650B or HP 1651B

Number of Probes Used: Two 16-channel probes

NSC 800 CPU Package: 40-pin DIP

**Accessories Required: HP 10303B Preprocessor
HP 10269C General Purpose Probe Interface**

Maximum Clock Speed: 4 MHz clock input

**Signal Line Loading: Maximum of one HCMOS load + 35 pF on any
line**

**Microprocessor Cycles Identified: Memory read/write
I/O read/write
Opcode fetch
Interrupt acknowledge
RAM refresh cycles
DMA cycles**

**Maximum Power Required: 0.1A at + 5 V dc, supplied by logic
analyzer**

Logic Analyzer Required: HP 1650B or HP 1651B

Number of Probes Used: Two 16-channel probes

8085 CPU Package: 40-pin DIP

**Accessories Required: HP 10304B Preprocessor
HP 10269C General Purpose Probe Interface**

Maximum Clock Speed: 6 MHz clock output (12 MHz clock input)

**Signal Line Loading: Maximum of one 74LS TTL load + 35 pF on any
line**

**Microprocessor Cycle Identified: Memory read/write
I/O read/write
Opcode fetch
Interrupt acknowledge**

**Maximum Power Required: 0.8 A at + 5 V dc, supplied by logic
analyzer**

Logic Analyzer Required: HP 1650B or HP 1651B

Number of Probes Used: Two 16-channel probes

8086 or 8088 CPU Package: 40-pin DIP

Accessories Required: HP 10305B Preprocessor
HP 10269C General Purpose Robe Interface

Maximum Clock Speed: 10 MHz clock input (at CLK)

Signal Line Loading: Maximum of two 74ALS TTL loads + 40 pF on any line

Microprocessor Cycles **Identified:** Memory read/write
I/O read/write
Code fetch
Interrupt acknowledge
Halt acknowledge
Transfer to 8087 or 8089 co-processors

Additional Capabilities: The 8086 or 8088 can be operating in Minimum or Maximum modes. The logic analyzer can capture all bus cycles (including prefetches) or can capture only executed instructions. To capture only executed instructions, the 8086 or 8088 must be operating in the Maximum mode.

Maximum Power Required: LO A at + 5 V dc, supplied by the logic analyzer

Logic Analyzer Required: HP 1650B

Number of Probes Used: Three 16-channel probes

80186 or **80C186** CPU Package: 68-pin PGA

Accessories Required: HP 10306G Preprocessor

Maximum Clock Speed: 12.5 MHz clock output (25 MHz clock input)

Signal Line Loading: Maximum of 100 k Ω + 18 pF on any line

Microprocessor Cycles Identified: Memory read/write (DMA and non-DMA)
I/O read/write (DMA and non-DMA)
Code fetch
interrupt acknowledge
Halt acknowledge
Transfer to 8087, 8089,
or 82586 co-processors

Additional Capabilities: The 80186 can be operating in Normal or Queue Status modes. The logic analyzer can capture all bus cycles (including prefetches) or can capture only executed instructions.

Maximum Power Required: 0.08 A at +5 V dc, supplied by system under test.

Logic Analyzer Required: HP 1650B

Number of Probes Used: Four 16-channel probes

80286 CPU Package: 68-contact LCC or 68-pin PGA

Accessories Required: HP 10312D Preprocessor
HP 10269C General Purpose Robe Interface

Maximum Clock Speed: 10 MHz dock output (20 MHz dock input)

Signal Line Loading: Maximum of two 74ALS TTL loads + 40 pF on any line

Microprocessor Cycles Identified: Memory read/write
I/O read/write
Code fetch
Interrupt acknowledge
Halt
Hold acknowledge
Lock
Transfer to 80287 co-processor

Additional Capabilities: The logic analyzer captures all bus cycles including prefetches

Maximum Power Required: 0.66 A at + 5 V dc, supplied by logic analyzer. 80286 operating current from system under test.

Logic Analyzer Required: HP 1650B

Number of Probes Used: Three 16-channel probes

80386 CPU Package: 132-pin PGA

Accessories Required: HP 10314B Preprocessor
HP 10269C General Purpose Probe Interface

Maximum Clock Speed: 20 MHz clock output (40 MHz clock input)

Signal Line Loading: Maximum of two 74ALS TTL loads + 35 pF on any line

Microprocessor Cycles Identified: Memory read/write
I/O read/write
code fetch
Interrupt acknowledge, type 0-255
Halt
Shutdown
Transfer to 8087, 80287, or 80387
co-processors

Additional Capabilities: The logic analyzer captures all bus cycles including prefetches

Maximum Power Required: 1.0 A at + 5 V dc, supplied by logic analyzer

Logic Analyzer Required: HP 1650B

Number of Probes Used: Five 16-channel probes

6800 or 6802 CPU Package: 40-pin DIP

Accessories Required: HP 10307B Preprocessor
HP 10269C General Purpose Probe Interface

Maximum Clock Speed: 2 MHz clock input

Signal Line Loading: Maximum of 1 74LS TTL load + 35 pF on any
line

Microprocessor Cycle Identified: Memory read/write
DMA read/write
Opcode fetch/operand
subroutine enter/exit
System stack push/pull
Halt
Interrupt acknowledge
Interrupt or reset vector

Maximum Power Required: 0.8A at + 5 V dc, supplied by logic
analyzer

Logic Analyzer Required: HP 1650B or HP 1651B

Number of Probes Used: Two 16-channel probes

6809 or 6809E CPU Package: **40-pin** DIP

Accessories Required: **HP 10308B Preprocessor**
HP **10269C** General **Purpose** Probe **Interface**

Maximum Clock Speed: 2 MHz clock input

Signal Line Loading: Maximum of one 74ALS TTL load + 35 pF on
ally line

Microprocessor **Cycles Identified:** Memory read/write
DMA read/write
Opcode fetch/operand
vector fetch
Halt
Interrupt

Additional Capabilities: The preprocessor can be adapted to **6809/09E**
systems that use a **Memory Management Unit**
(MMU). This adaptation allows the capture of
all address **lines** on a physical address bus up
to **24 bits wide**.

Maximum Power Required: 1.0 A at + 5 V dc, supplied by logic
analyzer

Logic Analyzer Required: HP **1650B** or **HP 1651B**

Number of Probes Used: Two **16-channel** probes

68008 CPU Package: 40-pin DIP

**Accessories Required: HP 10310B Preprocessor
HP 10269C General Purpose Probe Interface**

Maximum Clock Speed: 10 MHz clock input

**Signal Line Loading: Maximum of one 74S TTL load + one 74F TTL
load + 35 pF on any line**

**Microprocessor Cycles Identified: User data read/write
User program read
Supervisor read/write
Supervisor program read
Interrupt acknowledge
Bus grant
6800 cycle**

**Additional Capabilities: The logic analyzer captures all bus cycles
including prefetches**

**Maximum Power Required: 0.4 A at + 5 V dc, supplied by logic
analyzer**

Logic Analyzer Required: HP 1650B

Number of Probes Used: Three 16-channel probes

68000 and 68010 CPU Package: 64-pin DIP
(64-pin DIP)

Accessories Required: HP 10311B Preprocessor
HP 10269C General Purpose Probe Interface

Maximum Clock Speed: 12.5 MHz clock input

Signal Line Loading: Maximum of one 74S TTL load + one 74F
TTL load + 35 pF on any line

Microprocessor Cycles Identified: User data read/write
User program read
Supervisor read/write
Supervisor program read
Interrupt acknowledge
Bus Grant
6800 cycle

Additional Capabilities The logic analyzer captures all bus cycles
including prefetches

Maximum Power Required: 0.4 A at +5 V dc, supplied by the logic
analyzer

Logic Analyzer Required: HP 1650B

Number of Probes Used: Three 16-channel probes

**68000 and 68010
(68-pin PGA)**

CPU Package: **68-pin** PGA

Accessories Required: HP10311G Preprocessor

Maximum Clock Speed: 12.5 MHz clock input

Signal Line Loading: 100 k Ω + 10 pF on any line

Microprocessor Cycles Identified: User data read/write
User program read
Supervisor read/write
Supervisor program read
Interrupt acknowledge
Bus Grant
6800 cycle

Additional Capabilities: The logic analyzer captures all bus cycles including prefetches.

Maximum Power Required: None

Logic Analyzer Required: HP 1650B

Number of Probes Used: Three 16-channel probe4

68020 CPU Package: 114-pin PGA

Accessories Required: HP 10313G

Maximum Clock Speed: 25 MHz clock input

Signal Line Loading: 100 k Ω + 10 pF on any line

Microprocessor Cycles Identified: User data read/write
User program read
Supervisor read/write
Supervisor program read
Bus Grant
CPU space accesses including:
Breakpoint acknowledge
Access level control
Coprocessor communication
Interrupt acknowledge

Additional Capabilities The logic analyzer captures all bus cycles including prefetches. The 68020 microprocessor must be operating with the internal cache memory disabled for the logic analyzer to provide inverse assembly.

Maximum Power Required: None

Logic Analyzer Required: HP 1650B

Number of Probes Used: Five 16-channel probes

68030 CPU Package: 128-pin PGA

Accessories Required: HP 10316G

Maximum Clock Speed: 25 MHz input

Signal Line Loading: 100 K Ω plus 18 pF on all lines except DSACK0 and DSACKL

Microprocessor Cycles Identified: User data read/write
User program read
Supervisor program read
Bus grant
CPU space accesses including

Breakpoint acknowledge
Access level control
Coprocesor communication
Interrupt acknowledge

Additional Capabilities: The logic analyzer captures all bus cycles, including prefetches. The 68030 microprocessor must be operating with the internal cache memory and MMU disabled for the logic analyzer to provide inverse assembly.

Maximum Power Required: None

Logic Analyzer Required: HP 1650B

Number of Probes Used: Five 16-channel probes

68HC11 CPU Package: 48-pin dual-in-line

Accessories Required: HP 10315G

Maximum clock speed: 8.4 MHz input

Signal Line Loading: 100 K Ω plus 12 pF on all lines.

Microprocessor Cycles Identified: Data read/write
Opcode/operand fetches
Index offsets
Branch offsets
Irrelevant cycles

Additional Capabilities: The **68HC11** must be operating in the expanded multiplexed mode (addressing external memory and/or peripheral devices) for the logic analyzer to provide inverse assembly.

Maximum Power Required: None

Logic Analyzer Required: BP 1650B/51B

Number of Probes Used: Two 16-channel probes for state analysis and one to four for timing analysis.

Loading Inverse Assembler Files

you load the **inverse** assembler file by loading the **appropriate configuration** file. Loading the **configuration file** automatically loads the **inverse assembler file**.

Selecting the Correct File

Most **inverse assembler disks** contain more than one file. Each disk usually contains an **inverse assembler file** for use with the **HP 10269C** and **preprocessor** as well as a file for **general purpose probing**. Each **inverse assembler filename** has a **suffix** which indicates whether it is for the **HP 10269C** and **preprocessor** or **general purpose probing**. For example, filename **C68000_I** indicates a **68000 inverse assembler file** for use with the **HP 10269C** and the **68000 preprocessor**. Filename **C68000_P** is for **general purpose probing**. Specific **file descriptions** and **recommended usage** are **contained in** each **preprocessor operating note**.

Loading the Desired File

To load the **inverse assembler file** you want, insert the **3.5-inch disk** you received with your **preprocessor** in the **disk drive**. Select the **I/O menu**. In the **I/O menu**, select **DISK OPERATIONS**. The logic **analyzer** will read the disk and display the **disk directory**.

Select the **Load** option and **place** the **filename** you want to load in the **"from file" box**. Place the **cursor** on **Execute** and press **SELECT**.

Place the **cursor** on the **analyzer** you want the **file** loaded into and press **SELECT**. An advisory **"Loading file from disk"** is displayed. When the logic **analyzer** has finished loading the **file**, you will see "Load operation complete."

The file is now loaded and the logic analyzer **is** configured for **disassembly** of acquired data.

Connecting the Logic Analyzer Probes

The specific preprocessor and inverse assembler you are using determine how you connect the logic analyzer probes. Since the inverse assembler tiles configure the System Configuration, State Format Specification, and State Trace Specification menus, you must connect the logic analyzer probe cables accordingly so that the acquired data is properly grouped for inverse assembly. Refer to the specific inverse assembler operating note for the proper connections.

How to Display Inverse Assembled Data

The specific preprocessor and inverse assembler you are using determines how the inverse assembled data is displayed. When you press RUN, the logic analyzer acquires data and displays the State Listing menu.

The State Listing menu will display as much information about the captured data as possible. For some microprocessors, the display will show a completely disassembled state listing.

Some of the preprocessors and/or the microprocessors under test do not provide enough status information to disassemble the data correctly. In this case, you will need to specify additional information (i.e., tell the logic analyzer what state contains the first word of an opcode fetch). When this is necessary an additional field (INVASM) will appear in the top center of the State Listing menu (see below). This field allows you to point to the first state of an Op Code fetch.

```

68000STATE - State Listing Invasm      Minimum X-0:  0 s
markers Statistics Valid runs:      Maximum X-0:  0 s
16 of 16                               Average X-0:  0 s
  
```

Figure E-2. Inverse Assemble Field

For complete details refer to the Operating Note for the specific preprocessor.

Index

A

- absolute 10-9
- accumulate D-6, 11-6
- accuracy
 - time interval D-6
- acquisition
 - fields (state trace) 15-13
 - specifications D-7
- acquisition modes
 - glitch 10-5
 - state 15-13
 - timing 10-3
 - transitional 10-4
- activity indicators 12-5
- alpha entry 3-14
- alternate printers 7-2
- analyzer
 - configuration capabilities 1-2-1-3
 - type 4-4
- analyzers
 - How to Switch between 3-8
- armed by
 - state 15-13
 - timing 10-3
- arming D-7
- ASCII 9-9
- Assigning Pod Bits to Labels 3-17
- asynchronous pattern D-6
- Autoload 5-6, 6-1
 - disable 5-6
 - enable 5-6

- autoloading a file 6-U
- Autoscale 4-5, D-7
- Axes (State Chart)
 - Scaling the 18-2
 - Selecting the 18-1

B

- base 9-8, 10-6
 - ASCII 9-9
 - State Trace 15-22
- baud rate 516
- bit assignment 3-17, 9-4, 14-4
- BNCs
 - external trigger 3-6
- branches 15-14
 - per level 15-15
 - restart 15-14
- branching D-4
 - multiple levels 15-17
 - secondary 15-15
- branching qualifier 15-8

C

- cables
 - power B-4
 - printer 7-3
 - probe 2-6
- Cancel field 5-4
- channel-to-channel skew D-6

- CHS (change sign) key 3-4
- Clear Entry key 3 3
- clock D-3
 - demultiplex 14-10
 - master 14-10
 - mixed 14-11
 - normal 14-9
 - period (state) 14-12
 - pulse width D-1
 - qualifier D-3
 - repetition rate D-1
 - slave 14-10
 - state 14-7
- compare Image D-9,17-3
 - Bit Editing of the 17-4
 - boundaries D-9
 - Creating a 17-3
 - displays D-9
 - Masking Channels in the 17-5
 - stop measurement D-9
- Compare Images
 - Saving 17-8
- Compare Listing Display 17-2
- Compare Range 17-6
 - Specifying a 17-6
- configurations
 - analyzer 1-2-1-3, D-3
 - measurement D-3
- connecting
 - grabbers to probes 2-13
 - grabbers to test points 2-13
 - logic analyzer to target system 2-10
 - Other HP Printers 7-9
 - Pods to probe cable 2-11
 - probe cables to logic analyzer 2-10
- connectors
 - HP-IB Interface 3-7
 - pod cable 3-6
 - RS-232C Interface 3-6
- Continue field 5-4
- copy 5-7, 6-1
- Copying a File 6-15

- count 15-18
 - states 15-20
 - Time 15-18
- cursor 3-7

D

- data
 - bits 5-15
 - display D-8
 - entry D-8
 - How to Roll 316
 - time-correlating 22-u
- data entry
 - alpha 314
 - changing alpha entries 3-15
 - numeric 3-11
- Delay D-6
 - from Trigger (State) 19-5
- Delay (timing) II-9
- Deleting Waveforms (State) 19-4
- Demultiplex (clock) 14-10
- Difference Listing
 - Locating Mismatches in 17-8
- Difference Listing Display 17-2
- disable D4
- Disconnecting Probes from Pods 2-12
- disk
 - drive 3 5
 - drive operations 6-1
 - eject button 35
 - format (LIF) 6-7
 - indicator light 35
 - Installing a Blank Disk 6-6
 - operations 5-3
 - Removing Yellow Shipping Disk B-6
 - yellow shipping disk B-6
- disk operation parameters 6-5
- disk operations
 - Autoload 5-6, 6-1, 6-U

Index-2

HP 1650B/HP 1651B
Front-Panel Reference

- copy 5-7, 6-1
- Copying a File 6-15
- Duplicate Disk 5-8, 6-1
- Format Disk 5-11, 6-1
- Formatting a Disk 6-7
- load 5-5, 6-1, 6-11
- Pack Disk 5-9, 6-1
- Pack Disk Operation 6-17
- Purge 5-10, 6-1
- Purging a File 6-14
- Rename 5-9, 6-1
- Renaming a File 6-12
- Selectinga 6-4
- store 5-5, 6-1
- storing to a Disk 6-9
- Disk Operations menu
 - Accessing the 6-3
- display
 - key 33
 - Mixed Mode 21-1, 22-12
 - resolution (Timing Waveforms) 12-12
 - State/state Mixed Mode 21-3
 - time-correlated 21-4
 - Timing/State Mixed Mode 21-2
- display icons
 - The Inverted Triangle 12-11
 - Vertical Dotted Line 12-11
- Diilay Menu key 3-3
- Don't Care key 3-3
- Duplicate Disk 5-8, 6-1
- Duplicating the Operating System Disk 6-18

E

- ECL 2-9, 14-6
- edges
 - specifying 3-19
 - Then Find 10-11
- enable D-4
- entering data

HP 1650B/HP 1651B
Front-Panel Reference

- alpha 314
- changing alpha entries 3-15
- numeric 3-11
- error messages A-1
- Execute field 5-4
- external trigger BNCs 3-6
 - configuration 5-18

F

- fan 3-7
- file description 5-5, 6-9
- filename 5-5, 6-9
- Find Pattern 10-7
- Format Disk 5-11, 6-1
- Format Menu key 3-2
- Formatting a Disk 6-7
- Full Qualifier Specification 15-4
- fuse B-8

G

- glitch
 - minimum detectable width D-2
 - triggering 10-13
- Glitch Acquisition mode 10-5
- Glitch Capture mode D-5
- grabbers 2-7
- grounds
 - pod 2-7
 - power B-4
 - probes 2-8

H

- Hexadecimal keys 3-4
- hold time D-2

Hooking Up Your Printer 7-2

HP-IB

Interface connector 3-7

printer cables 7-3

I

I/O menu 5-1

Accessing the 5-1

I/O Menu key 3 3

I/O Port Configuration menu 5-12

indicators

activity D-7, 12-5

disk drive 3 5

markers D-7

trigger D-7

initial inspection B-1

installation B-1

Installation and Maintenance B-1

Installing a Blank Disk 6-6

intensity control B-10, 3-6

interface 3-1

Configuring 5-13

HP-IB 5-13, 7-1

RS-232C 5-14, 7-1

Setting HP-IB for HP Printers 7-4

Setting RS-232C for HP Printers 7-5

Setting RS-232C for Non-HP Printers 7-5

user 1-1, 3-1

inverse assembled data

How to Dii E-19

inverse assembler files

loading E-I.8

K

keys

CHS (change sign) 3-4

Clear Entry 3-3

Display Menu 33

Don't Care 33

Format Menu 32

Hexadecimal (HEX) 3-4

I/O Menu 3 3

menu 32

Roll 34, 316

Run 3 3

Select 3-4

stop 33

Trace-Menu 32

Knob 1-1, 3-4

L

Label Value vs. Label Value (State Chart) 18-4

Label Value vs. States (State Chart) 18-3

Labeling Pods, Probes, and Cables Z-14

labels D-7, 9-3

State Format Specification menu 14-3

State Trace 15-22

symbols 9-8

Timing Format Specification menu 9-3

Timing Trace Specification menu 10.6

line

power module B-7, 3-6

switch B-10, 3-6

voltage selector B-7, 3-6

Load 5-5, 6-1

loading a file 6-11

M

machine 31

machines 1-2

maintenance B-1

operator's B-12

- Making Hardcopy Prints 7-1
- marker functions D-8
 - Delta States D-8
 - patterns D-8
 - statistics D-8
 - time interval D-8
- markers
 - Pattern (state) 16-4
 - Pattern (timing) 11-5
 - Statistics (state) 16-6
 - Statistics (timing) 11-6
 - Time (state) 16-6
 - Time (timing) 11-4
 - Tii Waveforms menu 11-3
 - X and 0 12-10
- masterdock 14-10
- Maximum Probe Input voltage 2-9
- measurement example
 - state analyzer 20-1
 - timing analyzer 12-1
 - timing/state analyzer 22-1
- measurements
 - microprocessor E-1
- memory
 - acquisition D-3, 10-4-10-5
 - depth (glitch) D-5
- menu fields
 - How to Select 39
 - pop-up 3-9
 - Specify Symbols (state) 14-13
 - Specify Symbols (timing) 9-8
 - st/Div (states-per-c 19-4
 - State Format Specification 14-3
 - State Listing menu 16-3
 - State Trace menu 15-2
 - system configuration 43
 - Timing Format Specification 9-3
 - Timing Trace Specification 10-2
 - Timing Waveforms menu 11-3
 - toggle 3-11
- menu keys 3 2
- menu maps
 - state analyzer 13-1
 - state chart 13-9-13-10
 - State Compare 13-5
 - State Format 13-2
 - State Listing 13-4
 - State Trace 13-3
 - State Waveform 13-7-13-8
 - timing analyzer 8-1
 - Timing Format 8-2
 - Timing Trace 8-3
 - Timing Waveform 8-4
- menus
 - assignment/specification 3 1 7
 - Disk Operations 5-3, 6-1
 - How to Select 37
 - I/O 5-1
 - I/O Port Configuration 5-12
 - pop-up 3-9
 - Specify Symbols (state) 14-7, 14-12
 - Specify Symbols (timing) 9-7
 - State Chart 18-1
 - State Compare 17-1
 - State Format Specification 14-1
 - State Listing 16-1
 - State Trace 15-1
 - State Waveform 19-1
 - State Waveforms 19-1
 - System Configuration 4-1
 - system level 4-1
 - Timing Format Specification 9-1
 - Timing Trace Specification 10-1
 - Timing Waveforms 11-1
- mixed clocks 14-11
- mixed mode displays 21-1
 - Accessing the 21-1

N

- name
 - analyzer 3-14, 4-3

label 94,144
symbol **9-10**
numeric **entry** 3-q

O

0 to Trig(ger) 11-4
occurrence counter **D-4, 15-9**
operating **characteristics** D-2
operating environment B-2, D-10
Operating System
 Loading the B-8
operating system Disk 6-18
 Duplicating the 6-18
 Installing the B-9
overlapping Timing **Waveforms** 22-14
Overlaymode D-6

P

Pack Disk 5-9, 6-1
Packing a Disk 6-17
paper width 5-17
 Setting the 7 6
parity **5-15**
pattern
 recognizers **D-4, 15-2**
Pattern **Fields** (state) 1524
patterns **15-23**
 Duration (**present for**) **10-9**
 fields **15-22**
 find **10-7**
 specifying **3-18**
Pod Clock 14-9
pod threshold
 ECL **9-6**
 TTL **9-6**
 user-defined **9-6**

Pods **2-5, 4-6**
 cable connectors **3-6**
 clock 14-9
 ground 2-7
 probe pod assembly 2-5
 probes 2-5
 threshold **2-9, 9-6, 14-6**
Polarity (**Pol**) **9-4, 14-4**
pop-up
 How to Close 3-9
 How to **Select** (options) **3-10**
 menus 39
 options 110
power
 (line) switch B-10
 cable B-4
 cord **configurations** B-5
 ground B-4
 requirements B-3
preprocessors E-2
prestore **D-4, 15-21**
print
 An **5-2, 7-7**
 screen **5-2, 7-7**
 Starting the Printout 7-7
Print All **5-2, 7-7**
Print Screen **5-2, 7-7**
printer **5-16**
printers
 alternate 7-2
 Hooking Up 7-2
 Other HP Printers **7-9**
 supported 7-1
Probe Pod **Assembly** 2-5
probes **2-6**
 cable **2-6**
 dynamic range D-2
 ECL threshold preset D-2
 grabbers 2-7
 ground 2-8
 input RC D-2
 maximum input **voltage** 2-9

- maximum voltage** D-2
- minimum input overdrive** D-2
- minimum swing** D-1
- threshold **accuracy** D-1
- threshold range D-2
- threshold setting D-2
- TTL threshold** preset D-2
- Probes and Probe Pods 2-5
- probing**
 - general purpose 2-3
 - HP 1650B/51B System 2-5
 - options 2-1
 - termination** adapter 2-3
- protocol s-14
- Purge 5-10, 6-1
- Purging a File** 6-14

Q

- Qualifier** Field (state) 15-23
- qualifier D-4, 15-2
 - branching** 15-8
 - fields** 15-22
 - storage 15-8

R

- range**
 - recognizers** D-4, 15-2
- ranges** 15-24
- Rename 5-9, 6-1
- repetitive
 - trace mode (state) 15-U
 - trace mode (timing) 10-3
- Replacing **Waveforms** (State) 19-3
- Roll** keys 3-4, 3-16
- RS-232C**
 - default configuration 7-6

- Interface** connector 3-6
 - printer **cables** 7-3
 - recommended protocol** 7-6
 - setting for HP printers** 7-5
 - setting for non-HP printers** 7-5
- Run Function** D-8
- Run key** 3-3

S

- sample period** 11-3
 - glitch** D-5
 - transitional** D-5
- Select** key 3-4
- Selecting a Waveform (State) 19-2
- Selecting** an Address (HP-IB) 5-13
- self test C-1, 5-18
 - operator C-1
 - power-up B-11, C-1
- sequence levels D-4, 15-6
 - Delete Level** 15-7
 - Insert Level** 15-7
 - Reading the Display 15-11
- setup time** D-1
- signal line loading** 2-9
- single**
 - trace** mode (state) 15-13
 - trace mode (timing) 10-3
- skew
 - channel-to-channel** D-6
- slaveclock 14-10
- specifications** D-1
- Specifying Edges** 3-19
- Specifying Patterns** 3-18
- st/Div** (states-per-division) 19-1, 19-4
- state analyzer 13-1
 - An Overview** 13-1
 - menu maps** 13-1
- State Chart **Display** D-9
- State Chart menu 18-1

- Accessing the **18-1**
- Accumulate** D-9
- markers **D-9**
- statedock** 14-7
- State Compare menu
 - Accessing the** 17-2
- State Compare mode D-9
- State Format **Specification** menu **14-1**
 - Accessing the** 14-1
 - fields 14-3
- State Listing** menu **16-1**
 - Accessing the** 16-2
 - fields **16-3**
- state tagging **15-20**
- state Trace menu **15-1**
 - Accessing the** 15-2
 - fields **15-2**
- State Waveform **Display** D-9
- State Waveform **menu**
 - Accumulate** D-9
- State Waveforms menu **19-1**
 - Accessing the** 19-1
 - Delay D-9
 - markers D-10
 - maximum number of waveforms **D-10**
 - Overlay mode D-9
 - States/div** D-9
- State/State **Mixed Mode** **21-3**
- stop bits** 5-15
- Stop Function** D-8
- Stop key** 3-3
- Stop Measurement
 - state **16-5**
- Stop **Measurement** (timing) 11-5
- storage and hipping B-2
- storage macro** 15-9
- storage **qualification** D-4
- storage **qualifier** 15-8
- Store **5-5, 6-1**
- Store exception to disk
 - state 16-S
 - State **Compare** 17-7

- timing **11-6**
- Storing to a Disk** 6-9
- supported printers** 7-1
- switch**
 - line** (power) B-10
- symbols 9-7
 - base **9-8, 14-14**
 - label **9-8, 14-13**
 - name **9-10, 14-15**
 - number of D-5
 - pattern D-5
 - range D-S
 - specify (state)** 14-7
 - view **size** 9-10, **14-15**
- system **Configuration** menu 4-1
 - Accessing the** 4-2
 - Returning to** 3-8

T

- tagging **15-18**
 - state **D-4, 15-20**
 - time **D-4, 15-19**
- termination adapter 2-3
 - pinouts** 2-4
- Then **Find Edge** **10-11**
- threshold
 - pod **2-9, 9-6, 14-6**
- time tagging** 15-19
- time-correlated** data 22-U.
- time-correlated** displays **21-4**
- Time/Div** (time per division)
 - timing** 11-8
- timing**
 - Trace mode** 10-3
- timing analyzer** 8-1
 - An Overview** 8-1
 - menu maps** 8-1
- Timing** Format Specification menu 9-1
 - Accessing the** 9-1

base 10-6
fields 9-3
Timing Trace Specification menu 10-1
 Access&the 10-1
 fields 10-2
Timing Waveforms
 Overlapping 22-14
Timing Waveforms menu 11-1
 Accessing the 11-2
 At _____ Marker _____ **field** 11-7
 Delay field 11-9
Timing Waveforms Menu fields 11-3
Timing/State Mixed Mode 21-2
Trace Menu key 3-2
Transitional Acquisition mode D-5, 10-4
triggering
 glitch/edge D-6
TTL 2-9, 14-6

Y

Yellow Shipping Disk
 Removing the B-6

U

user interface 1-1, 3-1

V

ventilation B-2
view size
 symbol 9-10

X

X and O markers
 State Chart 18-5
 State Waveform 19-5
 Timing Waveforms 12-10
X to Trig(ger) 11-4

HP 1650B/HP 1651B
Front-Panel Reference

Index-S

