
User's Guide

Publication number E3468-97004
July 2000

For Safety information, Warranties, and Regulatory information, see the pages behind the index.

© Copyright Agilent Technologies 1994-2000
All Rights Reserved

Toshiba Tx19/39 Series Emulation


Toshiba Tx19/39 Series Emulation—At a Glance

This manual describes how to set up several Agilent Technologies emulation products: an emulation probe, an emulation module, and an emulation migration. These emulators provide a low-cost way to debug embedded software for Toshiba Tx19/39 Series microprocessor. The emulator lets you use the target processor's built-in background debugging features, including run control and access to registers and memory. A high-level source debugger can use the emulator to debug code running on the target system.

You can connect the emulator to an analysis probe or you can connect it to a debug port on the target system through the provided target interface module (TIM). The emulator can be controlled by a debugger on a host computer.

Emulation Probe

The emulation probe is a stand-alone emulator.

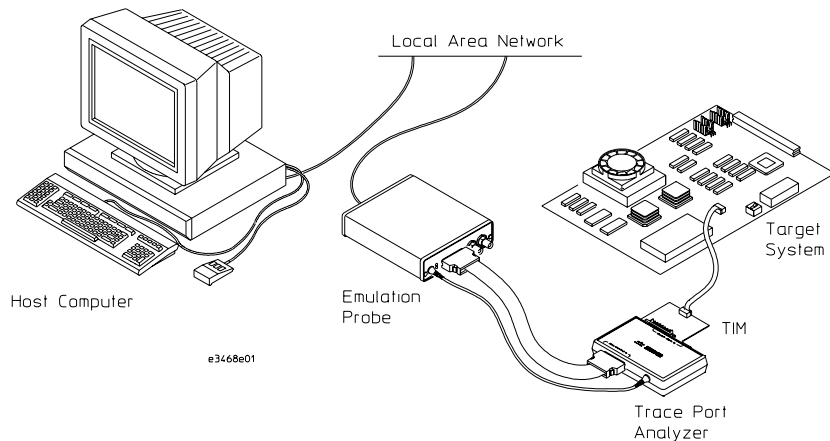


CAUTION


Trace Port Analyzer (E5903A#800) must be used with Emulation Probe.

Emulation Module

The emulation module plugs into your Agilent Technologies 16600A/700A-series logic analysis system frame.

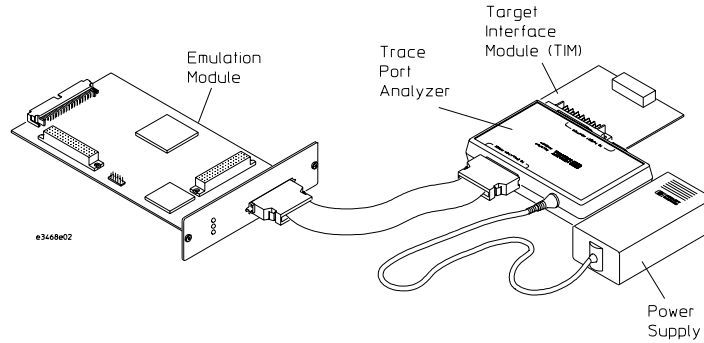

You can connect the emulation module to an analysis probe or you can connect it to a debug port on the target system through the provided target interface module (TIM).

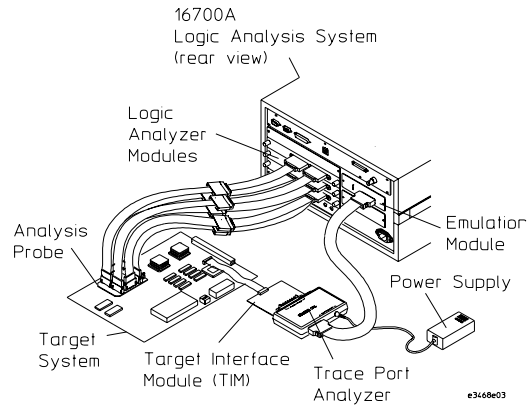

CAUTION

Trace Port Analyzer (E5903A#800) must be used with Emulation Probe.

Emulation Migration

The emulation migration includes a target interface module and firmware. Use the emulation migration if you already have an emulation probe or an emulation module for another processor.

In This Book

This book documents the following products:

Emulation Probe

Processors supported	Agilent Technologies Product ordered	Includes
TMPR 1904 TMPR 3901 TMPR 3903 TMPR 3904 Up to 75 MHz	E5900A Option #800	E3468A emulation probe, E3468A target interface module (TIM)

Emulation Module

Processors supported	Agilent Technologies Product ordered	Includes
TMPR 1904 TMPR 3901 TMPR 3903 TMPR 3904 Up to 75 MHz	E5901A Option #800	16610A emulation module, E3468A target interface module (TIM)

Emulation Migration

Processors supported	Agilent Technologies Product ordered	Includes
TMPR 1904 TMPR 3901 TMPR 3903 TMPR 3904 Up to 75 MHz	E5902A Option #800	E3468A target interface module (TIM)

Trace Port Analyzer

Processors supported	Agilent Technologies Product ordered	Includes
TMPR 1904 TMPR 3901 TMPR 3903 TMPR 3904 Up to 75 MHz	E5903A Option #800	E5890A Trace Port Analyzer

Contents

1 Overview 11

Setup Flowchart 13

Emulation Probe 14

- Equipment supplied 14
- Minimum equipment required 16
- To connect the emulation probe to a power source 16
- Emulation probe connection sequence 18

Emulation Module 19

- Equipment supplied 19
- Minimum equipment required 20

Trace Port Analyzer 21

- Equipment Supplied 21
- Minimum equipment required 22
- To connect a Trace Port Analyzer to a power source 23

Emulation Migration 24

- Equipment supplied 24

Minimum equipment required 25

Additional Information Sources 26

2 Connecting the Emulation Probe to a LAN 27

Setting Up a LAN Connection to a PC or Workstation 29

To obtain an IP address 30

To configure LAN parameters using the built-in terminal interface 31

To configure LAN parameters using BOOTP 34

To set the 10BASE-T configuration switches 36

To verify LAN communications 37

Setting Up a Serial Connection 38

To set the serial configuration switches 39

To connect a serial cable 39

To verify serial communications 41

3 Installing the Emulation Module 43

To install the emulation module in a 16700A-series logic analysis system or a 16701A expansion frame 45

To install the emulation module in a 16600A-series logic analysis system 47

4 Installing Software on a 16600A/700A 49

To list software packages which are installed (16600A/700A) 51

To install the software from CD-ROM (16600A/700A) 52

5 Connecting the Emulator 53

Designing a Target System 55

Wiring the N-wire 55

Precautions when you design your target system 57

Connecting the Emulator to the Target System 58

To connect to a target system using a debug port 59

To connect to a target system using an analysis probe 61

6 Updating Firmware 63

Emulation Probe Firmware 65

To display current firmware version information 65

To update firmware for an emulation probe 65

If there is a power failure during a firmware update 65

Emulation Module Firmware 66

To display current firmware version information 66

To update firmware for an emulation module using the Emulation Control Interface 66

To update firmware for an emulation module using the Setup Assistant 67

7 Specifications and Characteristics 69

Processor Compatibility 70

Emulation Probe Electrical Characteristics 71

Emulation Probe and Emulation Module Electrical Characteristics 72

Trace Port Analyzer Electrical Characteristics 72

Emulation Probe Environmental Characteristics 73

Emulation Module Environmental Characteristics 73
 Trace Port Analyzer Environmental Characteristics 73

8 Troubleshooting the Emulation Module 75

Emulation Module Troubleshooting Guide 77

Status Lights 78

Emulation Module Built-in Commands 81

To telnet to the emulation module 81
 To use the built-in commands 82

Problems with the LAN Interface (Emulation Probe Only) 84

If you cannot verify LAN communication 84
 If you have LAN connection problems 85
 If the "POL" LED is lit 86
 If it takes a long time to connect to the network 86

Problems with the Serial Interface (Emulation Probe Only) 87

If you cannot verify RS-232 communication 87
 If you have RS-232 connection problems with the MS Windows Terminal program 87

Problems with the Target System 89

What to check first 89
 To interpret the initial prompt 91

Problems with the LAN Interface 93

If LAN communication does not work 93
 If it takes a long time to connect to the network 94

Problems with the Emulation Probe 95
 To run the power up self test 95
 To execute the built-in performance verification test (emulation probe only) 97

Problems with the Emulation Module 102
 To run the built-in performance verification test using the logic analysis system (emulation module only) 102
 To run complete performance verification tests using a telnet connection (emulation module only) 103

Problem with the Trace Port Analyzer and TIM 105
 To perform the TIM and Trace Port Analyzer PV tests with an emulation probe/module 105
 To perform the TIM only PV tests with an emulation probe/module 106
 If a performance verification test fails 108

Returning Parts to Agilent Technologies for Service 109
 To return a part to Agilent Technologies 109
 To obtain replacement parts 110

Cleaning the Instrument 111

Glossary 113

Index 117


Overview

Overview

This chapter describes:

- Setup Checklist
- Equipment used with the emulation probe
- Connection sequences for the emulation probe
- Equipment used with the emulation module
- Additional information sources

Setup Flowchart

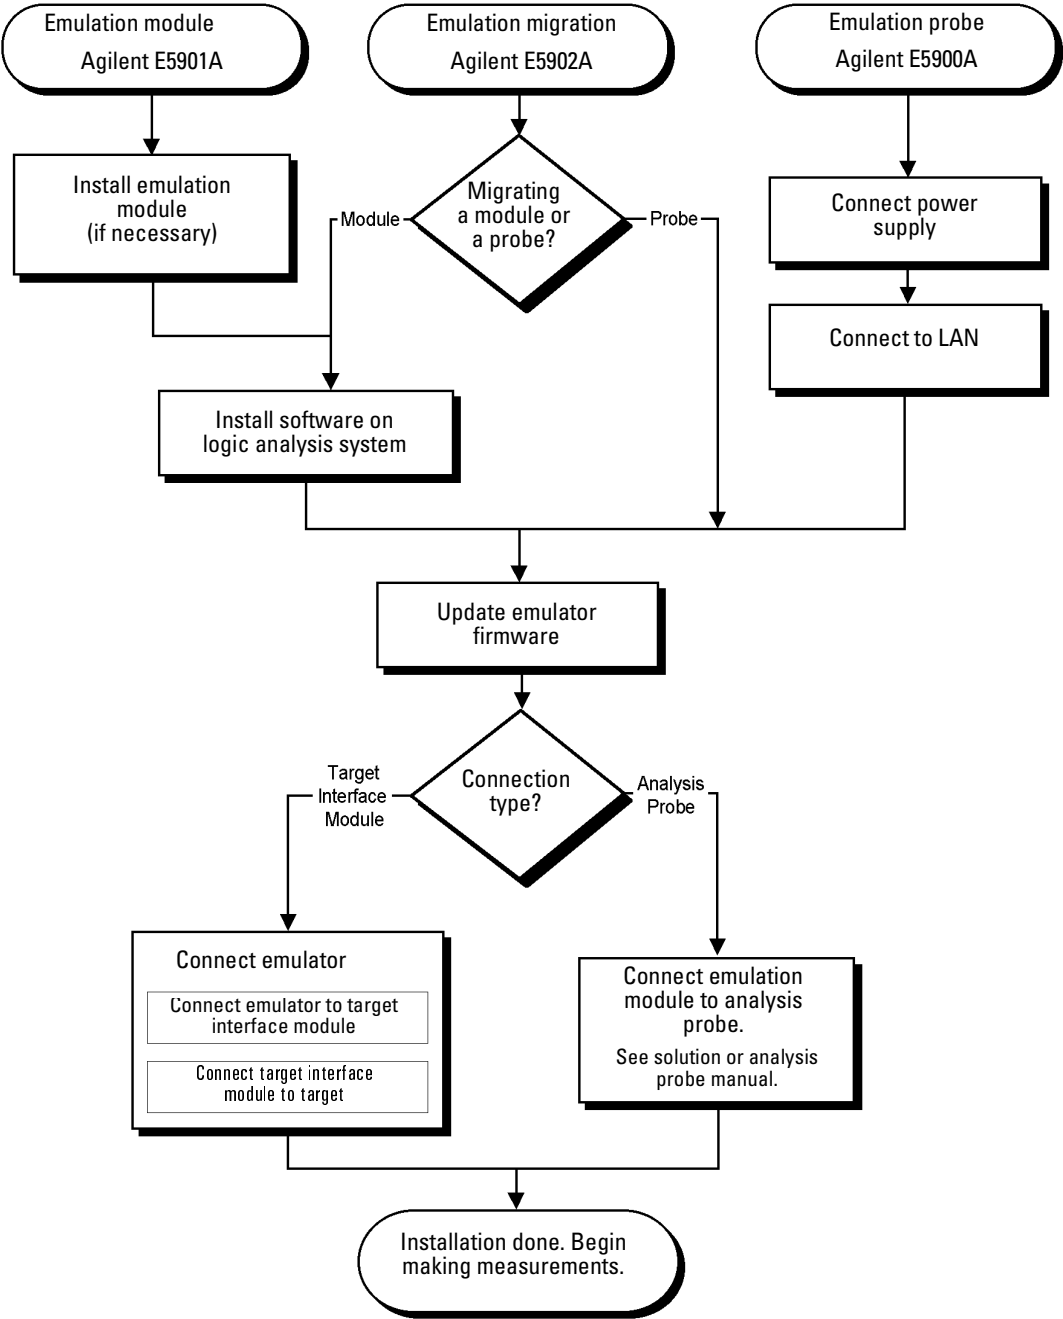


Emulation Probe

This section lists equipment supplied with the emulation probe and equipment requirements for using the emulation probe.

Equipment supplied

The equipment supplied with the emulation probe is shown in the illustration on the next page. It is listed below:

- An emulation probe.
- A 12V power supply for the emulation probe.
- A power cord.
- A target interface module (TIM) circuit board.
- A emulation module loopback test board (Agilent part number E3496-66502).
- A 50-pin ribbon cable for connecting the emulation module to the target interface module.
- A 20-pin ribbon cable for connecting the target interface module to the target system.
- This User's Guide.

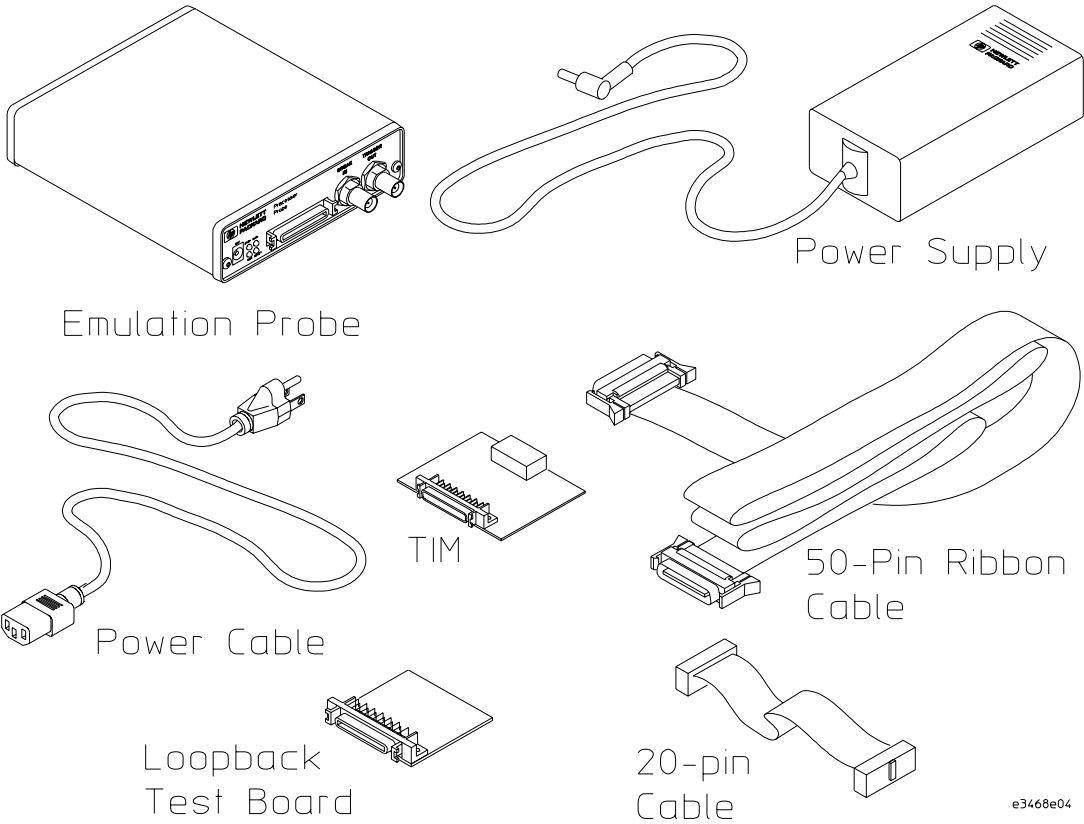

Equipment Supplied with Emulation Probe

e3468e04

Minimum equipment required

The following equipment is required to use the emulation probe:

- A method for connecting to the target system. The Agilent Technologies analysis probe provides a debug port connector. You can also design a debug port connector on the target system.
- A host computer, such as a PC or workstation.
- A LAN (local area network) to connect the emulation probe to the host computer.
- E5903A#800 Trace Port Analyzer
- A user interface on the host computer, such as B3759A#800 Emulation Solution Interface or 3rd party's high-level source debugger.

To connect the emulation probe to a power source

The emulation probe does not have an On/Off switch. To turn the emulation probe on or off, plug or unplug it from the power supply.

The emulation probe is shipped from the factory with a power supply and cord appropriate for your country. If the cord you received is not appropriate for your electrical power outlet type, contact your Agilent Technologies sales and service office.


Warning

Use only the supplied Agilent Technologies power supply and cord. Failure to use the proper power supply could result in electric shock.


Caution

Use only the supplied Agilent Technologies power supply and cord. Failure to use the proper power supply could result in equipment damage.

1 Connect the power cord to the power supply and to a socket outlet.

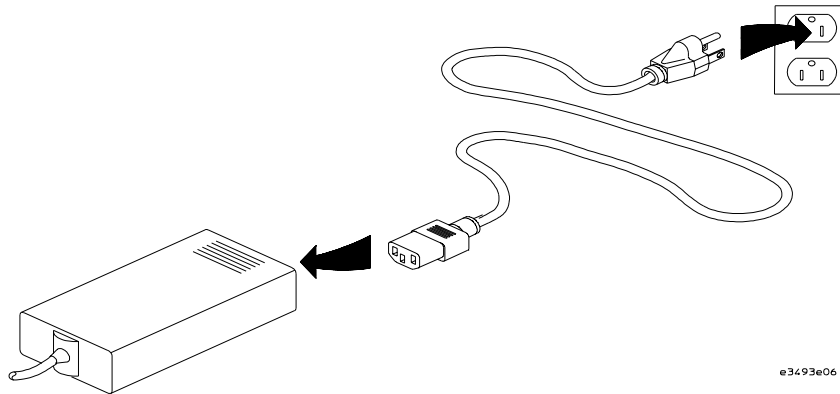

2 Connect the 12V power cord to the back of the emulation probe.

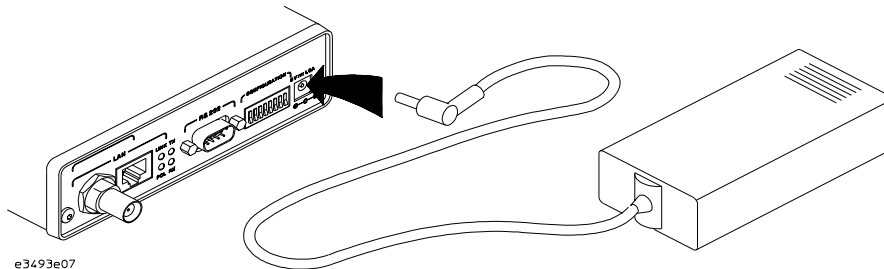

The power light on the target side of the emulation probe will light. The emulation probe does not have an On/Off switch.

With all components connected, power on your system in the following order:

- 1 Logic analyzer, if you are using one.
- 2 Emulation probe.
- 3 Your target system.

Power off your system in the following order:

- 1 Your target system
- 2 Emulation probe.
- 3 Logic analyzer, if you are using one.

Emulation probe connection sequence

Disconnect power from the target system, emulation probe, and logic analyzer before you make or break connections.

- 1 Connect the emulation probe to a LAN (page 27).
- 2 Connect the emulation probe to your target system (page 44).

Emulation Module


This section lists equipment supplied with the emulation module and lists the minimum equipment required to use the emulation module.

Equipment supplied

The equipment supplied with your emulation module includes:

- An Agilent Technologies 16610A emulation module. If you ordered an emulation module as part of your Agilent Technologies 16600A or 16700A logic analysis system, it is already installed in the frame.
- A target interface module (TIM) circuit board.
- A emulation module loopback test board (Agilent part number E3496-66502).
- Firmware for the emulation module on a CD-ROM.
- A 50-pin ribbon cable for connecting the emulation module to the target interface module.
- A 20-pin ribbon cable for connecting the target interface module to the target system.
- One Torx T-8, one Torx T-10, and one Torx T-15 screwdriver (if the emulation module was not installed at the factory).
- This User's Guide.

Chapter 1: Overview Emulation Module

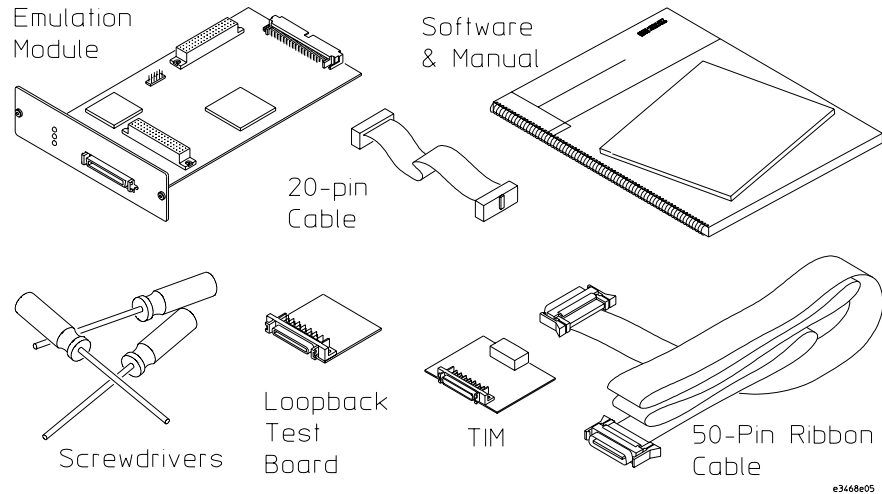

Equipment Supplied with the Agilent Technologies E3497A Emulation Module

Minimum equipment required

The following equipment is required to use the emulation module:

- A method for connecting to the target system. The Agilent Technologies analysis probe provides a debug port connector. You can also design a debug port connector on the target system.
- An Agilent Technologies 16600A or 16700A logic analysis system.
- E5903A#800 Trace Port Analyzer
- A user interface on the host computer, such as B3759A#800 Emulation Solution Interface or 3rd party's high-level source debugger .


Trace Port Analyzer

This section lists equipment supplied with the trace port analyzer and lists the minimum equipment required to use the trace port analyzer.

Equipment Supplied

The equipment supplied with your trace port analyzer includes:

- Trace Port Analyzer
- A 12V power supply
- DC-DC power code for connection with the Emulation probe
- A trace port analyzer loopback test board (Agilent part number: E5890-66502)

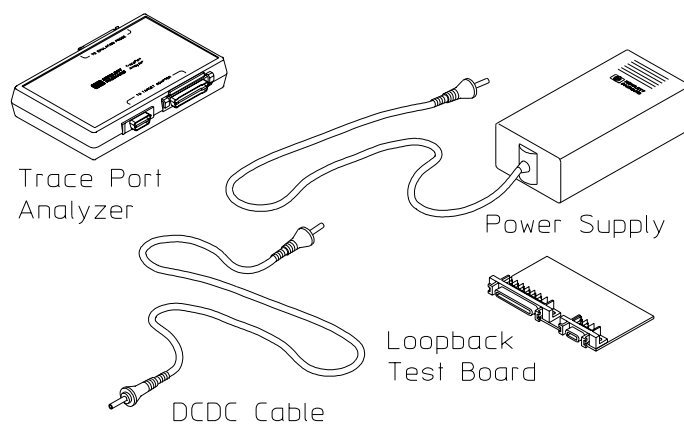


Minimum equipment required

The following equipment is required to use the trace port analyzer:


- An emulation module or emulation probe.
- A 50-pin data cable (supplied with the emulation module or probe).
- A method for connecting to the target system. The Agilent Technologies analysis probe provides a debug port connector. You can also design a debug port connector on the target system.
- A host computer such as a PC, a workstation, or an Agilent Technologies 16600A or 16700A logic analysis system.
- E5903A#800 Trace Port Analyzer

A user interface on the host computer, such as B3759A#800 Emulation Solution Interface or 3rd party's high-level source debugger .

To connect a Trace Port Analyzer to a power source

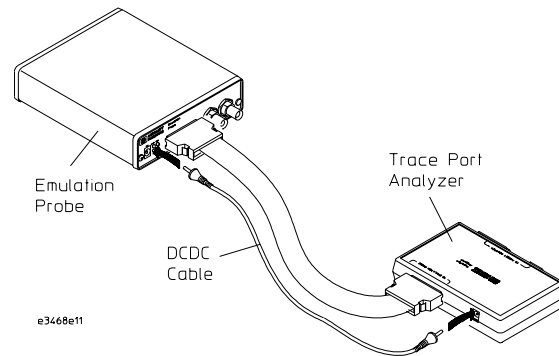

Connect a DC-DC power code before supplying a power to the emulation module.

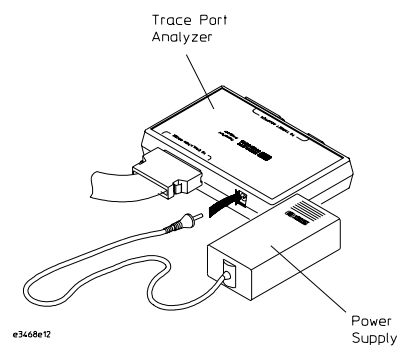

Power-On the logic analyzer or the emulation probe first, then connect power to the Trace Port Analyzer.


Emulation Migration

This section lists equipment supplied with the emulation migration and lists the minimum equipment required to use the emulation migration.

Equipment supplied

The equipment supplied with your emulation migration includes:

- A target interface module (TIM) circuit board.
- Firmware for the emulation module on a flexible disk.
- A 20-pin ribbon cable for connecting the target interface module to the target system.
- This User's Guide.

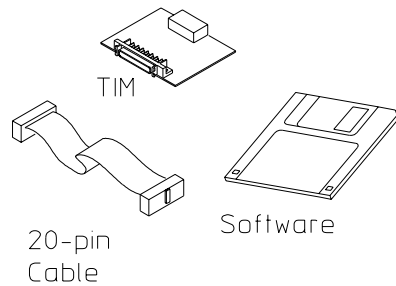

e3468e06

Minimum equipment required

The following equipment is required to use the emulation migration:

- An emulation module or emulation probe.
- A 50-pin data cable (supplied with the emulation module or probe).
- A method for connecting to the target system. The Agilent Technologies analysis probe provides a debug port connector. You can also design a debug port connector on the target system.
- A host computer such as a PC, a workstation, or an Agilent Technologies 16600A or 16700A logic analysis system.
- E5903A#800 Trace Port Analyzer
- A user interface on the host computer, such as B3759A#800 Emulation Solution Interface or 3rd party's high-level source debugger .

Additional Information Sources

Additional or updated information can be found in the following places:

Newer editions of this manual may be available. Contact your local Agilent Technologies representative.

If you have an analysis probe, the instructions for connecting the probe to your target microprocessor are in the analysis probe documentation. The ***Solutions for the Toshiba Tx19/39 Series User's Guide*** provides information on using the analysis probe and emulation module together.

Application notes may be available from your local Agilent Technologies representative or on the World Wide Web at:

<http://www.agilent.com/find/logicanalyzer>

The **measurement examples** include valuable tips for making emulation and analysis measurements. You can find the measurement examples under the system help in your Agilent Technologies 16600A/700A logic analysis system.

Connecting the Emulation Probe to a LAN

Connecting the Processor Probe to a LAN

You can connect your PC or workstation to the emulation probe via a serial or LAN connection.

Serial connection

A serial connection allows you to complete all of the performance verification tests. Other use of the serial port is not supported: performance over a serial connection, especially if you are downloading code, may be unacceptably slow.

LAN connection

A LAN connection will allow you to make your measurements quickly and easily. A few of the performance verification tests cannot be run over a LAN.


Recommended connection

Use a LAN connection for routine use, and a serial connection for LAN configuration and for troubleshooting.

Setting Up a LAN Connection to a PC or Workstation

The emulation probe has two LAN connectors:

- A BNC connector that can be directly connected to a IEEE 802.3 Type 10BASE2 cable (ThinLAN). When using this connector, the emulation probe provides the functional equivalent of a Medium Attachment Unit (MAU) for ThinLAN.
- An IEEE 802.3 Type 10BASE-T (StarLAN) connector.



Use either the 10BASE2 or the 10BASE-T connector. Do *not* use both. The emulation probe will not work with both connected at the same time.

You must assign an IP address (Internet address) to the emulation probe before it can operate on the LAN. You can also set other network parameters such as a gateway address. The IP address and other network parameters are stored in nonvolatile memory within the emulation probe.

The emulation probe automatically sets a subnet mask based on the subnet mask used by other devices on the network.

You can configure LAN parameters in any of the following ways:

- Using the built-in terminal interface over a serial connection. This is the most reliable method.
- Using BOOTP. BOOTP is part of the HP-UX, SunOS, and Solaris operating systems.

To obtain an IP address

- 1 Obtain the following information from your local network administrator or system administrator:

- An IP address for the emulation probe.

You can also use a "LAN name" for the emulation probe, but you must configure it using the integer dot notation (such as 127.0.0.1).

- The gateway address.

The gateway address is an IP address and is entered in integer dot notation. The default gateway address is 0.0.0.0, which allows all connections on the local network or subnet. If connections are to be made to workstations on other networks or subnets, this address must be set to the address of the gateway machine.

- 2 Find out whether port numbers 6470 and 6471 are already in use on your network.

The host computer interfaces communicate with the emulation probe through two TCP service ports. The default base port number is 6470. The second port has the next higher number (default 6471).

The default numbers (6470, 6471) can be changed if they conflict with some other product on your network.

To change the port numbers, see page 31. If you have already set the IP address, you can use a **telnet** connection instead of a serial connection to connect to the processor probe.

- 3 Write down the link-level address of the processor probe.

You will need this address if you use BOOTP to set the IP address.


The link-level address (LLA) is printed on a label above the LAN connectors on the emulation probe. This address is configured in each processor probe shipped from the factory and cannot be changed.

IP Address of Processor probe
LAN Name of Processor Probe
Gateway Address
Link-Level Address of Processor Probe

To configure LAN parameters using the built-in terminal interface

- 1 Set configuration switches S1 through S4 to CLOSED, and set the other switches as appropriate for your serial interface.

Switch settings are printed on the bottom of the emulation probe. If you will use a baud rate of 9600 baud, set the switches like this:

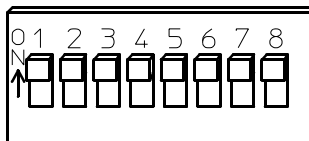

e3490b05

- 2 Connect an ASCII terminal (or terminal emulator) to the emulation probe's RS-232 port with a 9-pin RS-232 cable.
Complete instructions for setting up a serial connection begin on page 38.
- 3 Plug in the emulation probe's power cord. Press the terminal's <RETURN> key a couple times. You should see a prompt such as "p>", "?>", or "c>".
At this point, you are communicating with the emulation probe's built-in terminal interface.
- 4 Display the current LAN configuration values by entering the **lan** command:

```
R>lan
lan is disabled
lan -i 0.0.0.0
lan -g 0.0.0.0
lan -p 6470
Ethernet Address : 08000903212f
```

The "lan -i" line shows the current IP address (IP address) of the emulation probe.

The Ethernet address, also known as the link level address, is preassigned at the factory, and is printed on a label above the LAN connectors.

- 5 Enter the following command:

```
lan -i <internet> [-g <gateway>] [-p <port>]
```

The **lan** command parameters are:

-i <internet> The IP address which you obtained from your network administrator.

Chapter 2: Connecting the Emulation Probe to a LAN
Setting Up a LAN Connection to a PC or Workstation

-g <gateway> The gateway address. Setting the gateway address allows access outside your local network or subnet.

-p <port> This changes the base TCP service port number.
The default numbers (6470, 6471) can be changed if they conflict with some other product on your network. TCP service port numbers must be greater than 1024. If you change the base port, the new value must also be entered in the /etc/services file on the host computer. For example, you could modify the line:

```
hp64700    6470/tcp
```

The IP address and any other LAN parameters you change are stored in nonvolatile memory and will take effect the next time the processor probe is powered off and back on again.


- 6 Disconnect the power cord from the emulation probe, and connect the emulation probe to your network.

This connection can be made by using either the 10BASE-T connector or the 10BASE2 (BNC) connector on the emulation probe. Do not use both connectors at the same time.


- 7 Set the configuration switches to indicate the type of connection that is to be made.

Switch S1 must be set to OPEN, indicating that a LAN connection is being made.

Switch S5 should be CLOSED if you are connecting to the BNC connector:

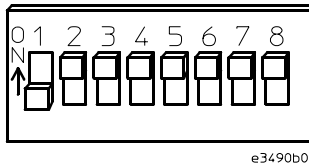

Switch S5 should be OPEN if you are connecting to the 10BASE-T connector:

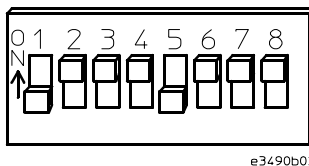

Set all other switches to CLOSED.

- 8 Connect the power cord to the emulation probe.

- 9 Verify your emulation probe is now active and on the network. See "To verify LAN communications" on page 37.

Once you have set a valid IP address, you can use the **telnet** utility to connect to the emulation probe, and use the **lan** command to change LAN parameters.

Example

To assign an IP address of 192.6.94.2 to the emulation probe, enter the following command:

```
R>lan -i 192.6.94.2
```

Now, cycle power on the emulation probe so that the new address will take effect.

See Also

"Solving Problems," page 75, if you have problems verifying LAN communication.

To configure LAN parameters using BOOTP

Use this method only on a workstation which is running **bootpd**, the BOOTP daemon.

1 Make sure that BOOTP is enabled on your host computer.

If the following commands yield the results shown below, the BOOTP protocol is enabled:

```
$ grep bootp /etc/services
bootps      67/udp
bootpc      68/udp
$ grep bootp /etc/inetd.conf
bootps dgram udp wait    root  /etc/bootpd  bootpd
```

If the commands did not yield the results shown, you must either add BOOTP support to your workstation or use a different method to configure the emulation probe LAN parameters.

2 Add an entry to the host BOOTP database file, `/etc/bootptab`. For example:

```
# Global template for options common to all Agilent Technologies
64700
# emulators and Processor Probes.
# Use a different gateway addresses if necessary.
hp64700.global:\
    :gw=0.0.0.0:\
    :vm=auto:\
    :hn:\
    :bs=auto:\
    :ht=ether

# Specific emulator entry specifying hardware address
# (link-level address) and ip address.
hprobe.div.hp.com:\
    :tc=hp64700.global:\
    :ha=080009090B0E:\
    :ip=192.6.29.31
```

In this example, the "ha=080009090B0E" identifies the link-level address of the emulation probe. The "ip=192.6.29.31" specifies the IP address that is assigned to the emulation probe. The node name is "hprobe.div.hp.com".

3 Connect the emulation probe to your network.


This connection can be made by using either LAN connector on the processor probe.

- 4 Set the configuration switches to indicate the type of connection that is to be made.


Switch S1 must be set to OPEN, indicating that a LAN connection is being made.

Switch S6 must be set to OPEN to enable BOOTP mode.

Switch S5 should be set to CLOSED if you are connecting to the BNC connector

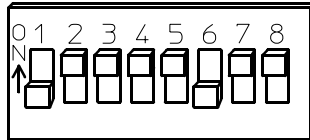

Switch S5 should be set to OPEN if you are connecting to the 10BASE-T connector.

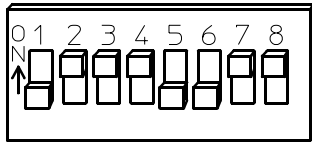

Set all other switches to CLOSED.

- 5 Connect the power cord to the emulation probe.
Verify that the power light stays on after 10 seconds.
The IP address will be stored in EEPROM.
- 6 Set switch S6 back to CLOSED.
Do this so that the emulation probe does not request its IP address each time power is cycled. The IP address is stored in EEPROM, so BOOTP does not need to be run again. Leaving this switch on will result in slower performance, increased LAN traffic, and even failure to power up (if the BOOTP server becomes inactive).
- 7 Verify your emulation probe is now active and on the network. See "To verify LAN communications" on page 37.

See Also

For additional information about using bootpd, refer to the bootpd (1M) man page.

To set the 10BASE-T configuration switches

Set switches S7 and S8 to CLOSED unless one of the following conditions is true:

- If the LAN cable exceeds the standard length, set switch S7 to OPEN.
The emulation probe has a switch-selectable, twisted-pair receiver threshold. With switch S7 set to OPEN, the twisted-pair receiver threshold is lowered by 4.5 dB. This should allow you to use cable lengths of up to about 200 meters. If you use a long cable, you should consult with your LAN cabling installer to ensure that:
 - The device at the other end of the cable has long cable capability, and
 - The cable is high-grade, low-crosstalk cable with crosstalk attenuation of greater than 27.5 dB.

When switch S7 is set to CLOSED, the LAN port operates at standard 10BASE-T levels. A maximum of 100 meters of UTP cable can be used.

- If your network doesn't support Link Beat integrity checking or if the emulation probe is connected to a non 10BASE-T network (such as StarLAN) set this switch to LINK BEAT OFF (0 or OPEN).

In normal mode (switch S8 set to CLOSED), a link integrity pulse is transmitted every 15 milliseconds in the absence of transmitted data. It expects to receive a similar pulse from the remote MAU. This is the standard link integrity test for 10BASE-T networks. If your network doesn't support the Link Beat integrity checking or if the Software Probe is used on a non 10BASE-T network (such as StarLAN) set this switch to LINK BEAT OFF (OPEN).

Note

Setting switch S8 to OPEN when Link Beat integrity checking is required by your network will cause the remote MAU to disable communications.

To verify LAN communications

- 1 Verify your emulation probe is now active and on the network by issuing a **telnet** to the IP address.

This connection will give you access to the emulation probe's built-in terminal interface.

- 2 To view the LAN parameters, enter the **lan** command at the terminal interface prompt.
- 3 To exit from this telnet session, type <CTRL>D at the prompt.

The best way to change the emulation probe's IP address, once it has already been set, is to telnet to the emulation probe and use the terminal interface **lan** command to make the change. Remember, after making your changes, you must cycle power or enter a terminal interface **init -p** command before the changes take effect. Doing this will break the connection and end the telnet session.

If You Have Problems

If you encounter problems, refer to the "Problems" chapter (page 75).

Example

```
$ telnet 192.35.12.6

R>lan
lan is enabled
lan -i 192.35.12.6
lan -g 0.0.0.0
lan -p 6470
Ethernet Address : 0800F090B30
```

Setting Up a Serial Connection

To set up a serial connection, you will need to:

- Set the serial configuration switches
- Connect a serial cable between the host computer and the emulation probe
- Verify communications

Serial connections on a workstation

If you are using a UNIX workstation as the host computer, you need to use a serial device file. If a serial device file does not already exist on your host, you need to create one. Once it exists, you need to ensure that it has the appropriate permissions so that you can access it. See the system documentation for your workstation for help with setting up a serial device.

Serial connections on a PC

Serial connections are supported on PCs. You must use hardware handshaking if you will use the serial connection for anything other than setting LAN parameters.

If you are using a PC as the host computer, you do not need to set up any special files.

To set the serial configuration switches

- 1 Set switch S1 to CLOSED (RS-232).
- 2 Set switches S2-S4 to CLOSED.
- 3 Set switch S5 to CLOSED (HW HANDSHAKE ON) if your serial interface uses the DSR:CTS/RTS lines for flow control. Set S5 to OPEN (HW HANDSHAKE OFF) if your serial interface uses software flow control (XON/XOFF).


If your serial interface supports hardware handshaking, you should use it (set switch S5 to CLOSED). Hardware handshaking will make the serial connection much more reliable.

- 4 Set switches S6-S8 for the baud rate you will use. These switch settings are listed on the bottom of the emulation probe.

The higher baud rates may not work reliably with all hosts and user interfaces. Make sure the baud rate you choose is supported by your host and user interface.

Example

To use a baud rate of 9600 baud, set the switches as follows:

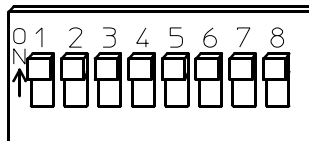

e3490b05

To connect a serial cable


CAUTION

Use a grounded, shielded cable. If the cable is not shielded, or if the cable is not grounded at the serial controller, the emulation probe may be damaged by electrostatic discharge.

Connect an RS-232C modem cable from the host computer to the processor probe. The recommended cable is Hewlett-Packard part number C2932A. This is a 9-pin cable with one-to-one pin connections.

Chapter 2: Connecting the Emulation Probe to a LAN
Setting Up a Serial Connection

If you want to build your own RS-232 cable, follow the pinout shown in the following figure:



Serial Cable Pinout

Pin Number	Signal	Signal Description
1	DCD	Data Carrier Detect (not used)
2	TD	Transmit Data (data coming from Agilent Technologies emulation probe)
3	RD	Receive Data (data going to Agilent Technologies emulation probe)
4	DTR	Data Terminal Ready (not used)
5	GND	Signal Ground
6	DSR	Data Set Ready (Output from Agilent Technologies emulation probe)
7	RTS	Request to Send (Input to Agilent Technologies emulation probe)
8	CTS	Clear to Send (connected to pin 6)
9	RING	Ring Indicator (not used)

To verify serial communications

- 1 Start a terminal emulator program on the host computer.
If you are using a PC, the Terminal application in Microsoft Windows will work fine.
If you are using a UNIX workstation, you can use a terminal emulator such as **cu** or **kermit**.
- 2 Plug the power cord into the emulation probe.
When the emulation probe powers up, it sends a message (similar to the one that follows) to the serial port and then displays a prompt:

```
Copyright (c) Agilent Technologies 1987  
All Rights Reserved.  Reproduction, adaptation, or translation without prior  
written permission is prohibited, except as allowed under copyright laws.
```

```
E3499A Series Emulation System  
Version:  A.07.06 06May97  
Location:  Generics
```

```
E3468A Toshiba Tx19/39 Series Emulator  
Version:  A.01.00 ????
```

R>

The version numbers may be different for your emulation probe.

- 3 Press the Return or Enter key a few times.
You should see a prompt such as "p>", "C>", or "?>".
For information about the commands you can use, enter ? or help at the prompt.

See Also "Problems with the Serial Interface," page 87.

Chapter 2: Connecting the Emulation Probe to a LAN
Setting Up a Serial Connection

Installing the Emulation Module

Installing the Emulation Module

This chapter shows you how to install an emulation module in your Agilent Technologies 16600A/700A-series logic analysis system.

If your emulation module is already installed in your logic analysis system frame, you may skip this chapter.

CAUTION


These instructions are for trained service personnel. To avoid dangerous electric shock, do not perform any service unless qualified to do so. Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

Electrostatic discharge can damage electronic components. Use grounded wriststraps and mats when you handle modules.


To install the emulation module in a 16700A-series logic analysis system or a 16701A expansion frame

You will need T-10 and T-15 Torx screw drivers.


- 1 Turn off the logic analysis system and **REMOVE THE POWER CORD**. Remove any other cables (such as probes, mouse, or video monitor).
- 2 Turn the logic analysis system frame upside-down.
- 3 Remove the bottom cover.

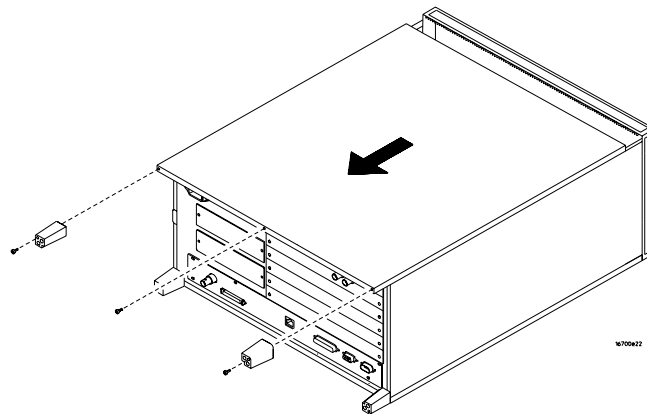

- 4 Remove the slot cover.
You may use either slot.

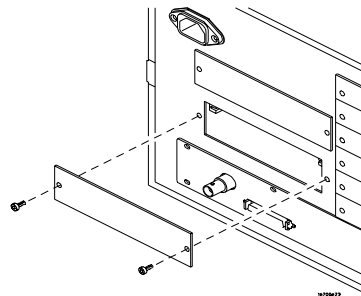


5 Install the emulation module.

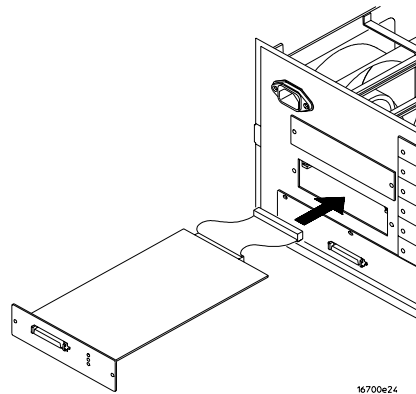

6 Connect the cable and re-install the screws.

You may connect the cable to either of the two connectors. If you have two emulation modules, note that many debuggers will work only with the "first" module: the one toward the top of the frame ("Slot 1"), plugged into the connector nearest the back of the frame.

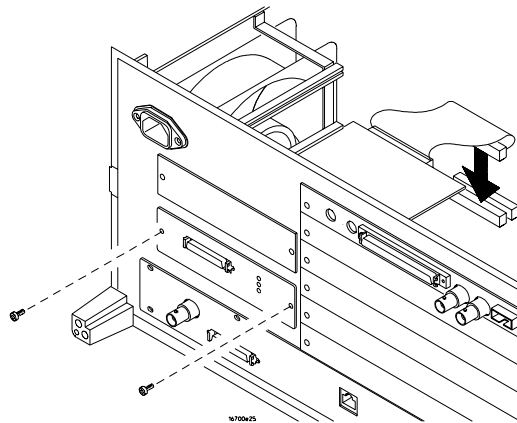

7 Reinstall the bottom cover, then turn the frame right-side-up.

8 Plug in the power cord, reconnect the other cables, and turn on the logic analysis system.

The new emulation module will be shown in the system window.


See Also

See page 63 for information on giving the emulation module a "personality" for your target processor.


To install the emulation module in a 16600A-series logic analysis system

You will need T-8, T-10, and T-15 Torx screw drivers.


- 1 Turn off the logic analysis system and **REMOVE THE POWER CORD**. Remove any other cables (such as probes, mouse, or video monitor).
- 2 Slide the cover back.

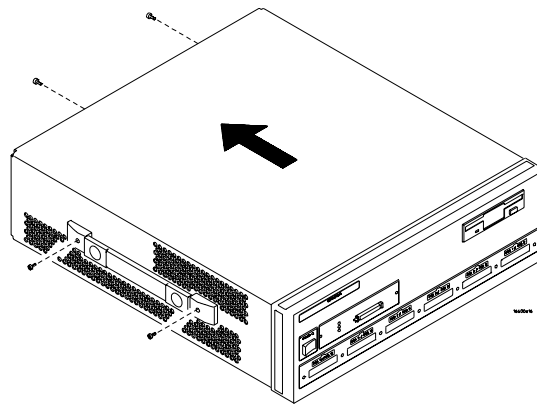

- 3 Remove the slot cover.

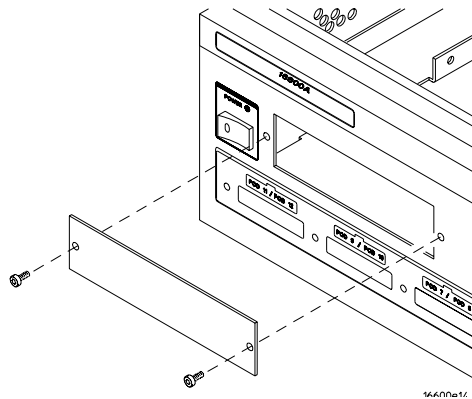

- 4 Install the emulation module.
- 5 Connect the cable and re-install the screws.

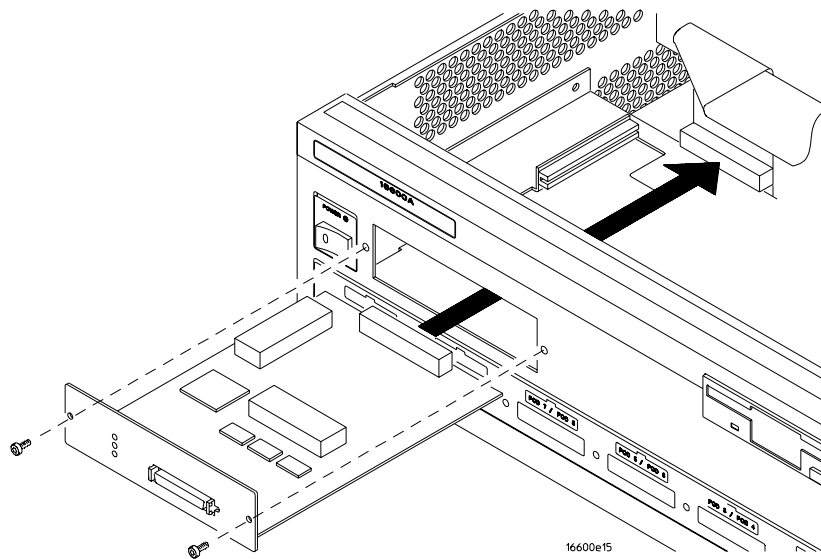

- 6 Reinstall the cover.
Tighten the screws snugly (2 N²m or 18 inch-pounds).
- 7 Plug in the power cord, reconnect the other cables, and turn on the logic analysis system.
The new emulation module will be shown in the system window.

See Also

See page 63 for information on giving the emulation module a "personality" for your target processor.


Installing Software on a 16600A/700A

Installing Software on a 16600A/700A

This chapter explains how to install the software you will need for your analysis probe or emulation solution.

Installing and loading

Installing the software will copy the files to the hard disk of your logic analysis system. Later, you will need to **load** some of the files into the appropriate hardware module.

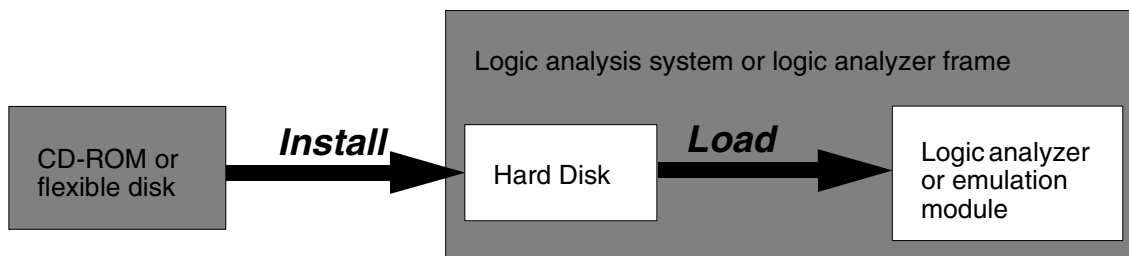

What needs to be installed

Agilent Technologies 16600A/700A-series logic analysis systems

If you ordered an emulation solution with your logic analysis system, the software was installed at the factory.

The following files are installed when you install a processor support package from the CD-ROM:

- Logic analysis system configuration files (not released yet)
- Personality files for the Setup Assistant
- Emulation module firmware

To list software packages which are installed (16600A/700A)

- In the System Administration Tools window, click **List...** .

To install the software from CD-ROM (16600A/700A)

Installing a processor support package from a CD-ROM will take just a few minutes. If the processor support package requires an update to the Agilent Technologies 16600A/700A operating system, installation may take approximately 15 minutes. If the CD-ROM drive is not connected, see the instructions printed on the CD-ROM package.

- 1 Turn on the CD-ROM drive first and then turn on the logic analysis system.
- 2 Insert the CD-ROM in the drive.
- 3 Click the **System Admin** icon.
- 4 Click **Install...**
Change the media type to "CD-ROM" if necessary.
- 5 Click **Apply**.
- 6 From the list of types of packages, select "PROC-SUPPORT."
A list of the processor support packages on the CD-ROM will be displayed.
- 7 Click on the "Tx19/39" package.
If you are unsure if this is the correct package, click Details for information on what the package contains.
- 8 Click **Install...**
The dialog box will display "Progress: completed successfully" when the installation is complete.
- 9 Click **Close**.

The configuration files are stored in `/hplogic/configs/hp/processor`.

The inverse assemblers are stored in `/hplogic/ia`.

See Also

The instructions printed on the CD-ROM package for a summary of the installation instructions.

The online help for more information on installing, licensing, and removing software.

Connecting the Emulator

Connecting the Emulator

This chapter shows you how to connect the emulator to the target system and how to configure the emulator and target processor.

Overview

Here is a summary of the steps for connecting and configuring the emulator:

- 1 Make sure the target system is designed to work properly with the emulator. (Page 55.)
- 2 Install the emulation module in your logic analysis system, if necessary. (Page 43.)
If you are connecting an emulation module to an Agilent Technologies 16600A/700A-series logic analysis system, use the Setup Assistant to guide you through steps 3-4.
- 3 Connect the emulator to your target system using the 50-pin cable and the TIM or an analysis probe. (Page 58.)
- 4 Update the firmware of the emulator, if necessary. (Page 63.)

Designing a Target System

This section will help you design a target system that will work with the Agilent Technologies E5900A #800 Emulation Probe.


Wiring the N-wire

To connect the Agilent Technologies E5900A #800 Emulation Probe to your target system, you have to prepare the following 20 signals called N-wire on your target system using the 20-pin connector.

N-wire

Cable Pin Number	Signal	TMPR3901F Pin Number
1	RESET	80
3	V _{DD}	79
5	DRESET	78
7	SDI/DINT	77
9	DBGE	76
11	SDA0/TPC	76
13	PCST[0]	74
15	PCST[1]	73
17	PCST[2]	72
19	DLCK	71
Odd Pins	V _{SS}	70 and others

Pin assignments for 20-pin connector is the following.

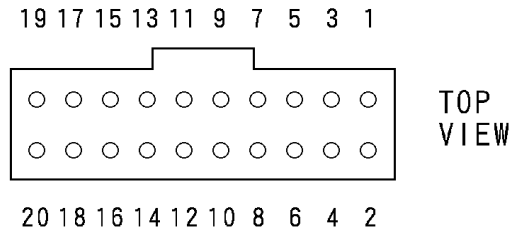

20-pin connector

You can use following connectors.

Supplier	Product Number	Description
AMP	104069-1	Shrouded - Right Angle
AMP	104068-1	Shrouded - Vertical
AMP	104549-2	Shrouded - Vertical (SMT)

Caution

Locate the 20-pin connector within 10cm (4 inches) from the microprocessor on your target system. If the 20-pin connector is located further than 10cm (4 inches) away from the microprocessor, Agilent Technologies E5900A #800 Emulation Probe may not work correctly.

Target V_{DD}

The Agilent Technologies E5900A #800 Emulation Probe may draw up to 10 mA from target V_{DD} .

Precautions when you design your target system

You need to pay attention to the following limitations when you design your target system.

Caution

While the monitor program is running, the processor's memory access cycles to the monitor area (0xff200000 - 0xff3fffff) cause bus cycles to be driven to the target system. You need to design your target system so that it may not cause errors such as address error at such bus cycles. Refer to the processor manual for the details. See "Glossary" for "monitor program".

Caution

You can NOT use debug functions of Tx19/39 series microprocessor, since these functions are reserved for the Agilent Technologies E5900A#800 emulation probe only.

Connecting the Emulator to the Target System

Choose one of the following methods for connecting the emulator to a target system.

- Directly through a debug port connector on the target board.
- Through an Agilent Technologies E**** (not released yet) analysis probe, which provides a direct connection to the debug port pins.

After you have connected the emulator to your target system, you may need to update the firmware in the emulator.

See Also


For information on designing a debug port on your target board, see page 55.

For a list of the parts supplied with the emulator, see page 19.


To connect to a target system using a debug port

The emulator can be connected to a target system through a 10-pin debug port (BDM connector). The emulator should be connected to a 10-pin male 2x5 header connector on the target system using the 10-conductor cable assembly provided.

- 1 Turn off the target system and disconnect it from all power sources.
- 2 Plug one end of the 50-pin cable into the emulator.



- 3 Plug the other end of the 50-pin cable into the Trace Port Analyzer.
- 4 Plug the target interface module into the Trace Port Analyzer.
- 5 Plug one end of the 20-pin cable into the target interface module.
- 6 Plug the other end of the 20-pin cable into the debug port on the target system.



- 7 Turn on the power to the logic analysis system and then the target system.

See Also


"Designing a Target System" (page 55) for information on designing a target system for use with the emulator.

Note

To lock connectors

The Trace Port Analyzer has a aligning lock to prevent the TIM from being disconnected.

1. Loosen the two screws
2. Slide a lock out as shown
3. Connect the TIM.
4. Slide lock in
5. Tighten the screws

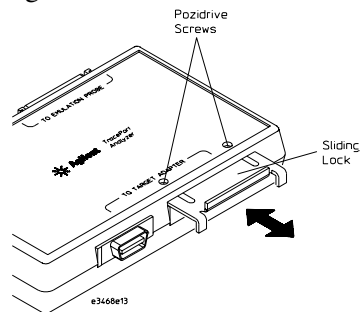

To connect to a target system using an analysis probe

Note To be described in future.

Updating Firmware

Updating Firmware

Firmware gives your emulator a “personality” for a particular processor or processor family.

After you have connected the emulator to your target system, you may need to update the firmware to give it the right personality for your processor.

You must update the firmware if:

- You have an emulation module which was not shipped already installed in the logic analysis system.
- You need to change the personality of the emulator for a new processor.
- You have an updated version of the firmware from Agilent Technologies.

The procedure for updating firmware for an emulation probe is different from the procedure for updating firmware for an emulation module.

Emulation Probe Firmware

To display current firmware version information

- Use telnet or a terminal emulator to access the built-in "terminal interface" and use the ver command to view the version information for firmware currently in the emulation probe.
-

To update firmware for an emulation probe

To update the firmware, you must have access to the World Wide Web and a PC or a workstation connected to your emulation probe.

- 1 Download the new firmware from the following World Wide Web site:

<http://www.agilent.com/find/emulator>

The firmware will be in the "Technical Support Information" section of this web site.

- 2 Follow the instructions on the web site for installing the firmware.

If Agilent Technologies sends you firmware on a floppy disk, install the firmware from the floppy disk. The README file on the floppy disk contains instructions for installing the firmware using a PC or workstation.

If there is a power failure during a firmware update

If there is a power glitch during a firmware update, some bits may be lost during the download process, possibly resulting in an Agilent Technologies processor probe that will not boot up.

- Set switch S4 to OPEN, then cycle power. This tells the Agilent Technologies processor probe to ignore everything in the Flash EPROM except the boot code.
 - Repeat the firmware update process.
 - Set switch S4 to CLOSED, then cycle power. This restores the Agilent Technologies processor probe to its normal mode.
-

Emulation Module Firmware


Always update firmware by installing a processor support package. This will ensure that the version of the Emulation Control Interface software is compatible the version of the emulator firmware.

To display current firmware version information

- 1 In the Update Firmware window, click Display Current Version.
There are usually two firmware version numbers: one for “Generics” and one for the personality of your processor.
-

To update firmware for an emulation module using the Emulation Control Interface

- 1 End any run control sessions which may be running.
- 2 In the Workspace window, remove any Emulator icons from the workspace.
- 3 Install the processor support package from the CD-ROM, if necessary.
- 4 In the system window, click the emulation module and select **Update Firmware...**

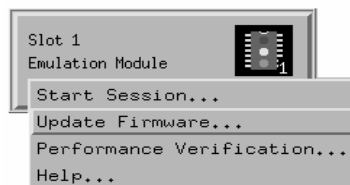

To update firmware for an emulation module using the Setup Assistant

- 5 In the Update Firmware window, select the firmware to load into the emulation module.
- 6 **Click Update Firmware.**
In about 20 seconds, the firmware will be installed and the screen will update to show the current firmware version.

See Also

“Installing Software” beginning on page 38 for instructions on how to install the processor support package from the CD-ROM.


To update firmware for an emulation module using the Setup Assistant

The Setup Assistant is an online tool for connecting and configuring your logic analysis system for microprocessor and bus analysis. The Setup Assistant is available on the Agilent Technologies 16600A and 16700A-series logic analysis systems.

This menu-driven tool will guide you through the connection procedures for connecting the logic analyzer to an analysis probe, an emulation module, or other supported equipment. It will also guide you through connecting an analysis probe to the target system.

Do not use the Setup Assistant to connect an emulation probe if you already have an emulation module installed.

- 1 Install the processor support package from the CD-ROM.
- 2 Start the Setup Assistant by clicking its icon in the system window.



- 3 Follow the instructions displayed by the Setup Assistant.

See Also

Page 51 for instructions on how to install a the processor support package from the CD-ROM.

To update firmware for an emulation module using the Setup Assistant

Specifications and Characteristics

The following operating characteristics are not specifications, but are typical operating characteristics for the Agilent Technologies 16610A emulation module, emulation probe, and Tx19/39 target interface module.

Processor Compatibility

The Agilent Technologies E3468A Tx19/39 Series emulator supports the TMPR 1904, 3901, 3903 and 3904 microprocessors.

Emulation Probe Electrical Characteristics

BNC, labeled TRIGGER OUT

Output Drive

Logic high level with 50-ohm load ≥ 2.0 V. Logic low level with 50-ohm load ≤ 0.4 V. Output function is selectable by the Agilent Technologies 16505A Prototype Analyzer. Refer to Online Help for more information.

BNC, labeled BREAK IN

Input

Edge-triggered TTL level input (active high), 20 pf, with 2K ohms to ground in parallel. Maximum input: 5 V above V_{CC} ; 5 V below ground. Input function is selectable by the Agilent Technologies 16505A Prototype Analyzer. Refer to Online Help for more information. The BNC introduces approximately 2.5 ms skid after break-in at 25 MHz.

Communications

Serial Port

9-pin female type “D” subminiature connector. RS-232 DCE to 115.2 kbaud.

10BASE-T LAN Port

RJ-45 connector. IEEE 802.3 10BASE-T (StarLAN).

10BASE 2 LAN Port

50-ohm BNC connector. IEEE 802.3 10BASE2 (ThinLAN). When using this connector, the emulation probe provides the functional equivalent of a Medium Attachment Unit (MAU) for ThinLAN.

Accessory Power Out

12 V, 3.0A, center negative

Power Supply

Input

100-240 V, 1.0 A, 50/60 Hz, IEC 320 connector.

Output

12 V, 3.3 A

Emulation Probe and Emulation Module Electrical Characteristics

Maximum Ratings

Characteristics for the Tx19/39 Embedded MIPS	Notes	Symbol	Min	Max	Unit
Input voltage range		V_{in}	-0.5	5.5	V
Input voltage range (V _{tt})			1.3	1.7	V
Input High Voltage		V_{ih}	$\frac{2}{3}V_{tt} + 0.2$		V
Input Low Voltage		V_{il}		$\frac{2}{3}V_{tt} - 0.2$	V
Input High Current		I_{ih}		-15	mA
Input Low Current		I_{il}		100	mA
Output High Voltage		V_{oh}	2.4	3.3	V
Output Low Voltage		V_{ol}		0.5	V
Output High Current		I_{oh}	8		mA
Output Low Current		I_{ol}	-16		mA

Trace Port Analyzer Electrical Characteristics

Characteristics for the Tx19/39 Trace Port Analyzer	Notes	Symbol	Min	Max	Unit
Input voltage range			-0.5	5.5	V
Input High Voltage			2.0		V
Input Low Voltage				0.7	V
Input High Current				-32	mA
Input Low Current				32	mA
Output High Voltage			2.4		V
Output Low Voltage				0.45	V
Output High Current			25		mA
Output Low Current			-25		mA

Emulation Probe Environmental Characteristics

Temperature

Operating, 0 to +40 °C (+32 to +104 °F); nonoperating, -40 to +60 °C (-40 to +140 °F).

Altitude

Operating/nonoperating 4600 m (15 000 ft).

Relative Humidity

15% to 95%.

For indoor use only.

Emulation Module Environmental Characteristics

The Agilent Technologies 16610A emulation module meets the environmental characteristics of the logic analysis system in which it is installed.

For indoor use only.

Trace Port Analyzer Environmental Characteristics

Temperature

Operating, 0 to +40 °C (+32 to +104 °F); nonoperating, -40 to +60 °C (-40 to +140 °F).

Altitude

Operating/nonoperating 4600 m (15 000 ft).

Relative Humidity

15% to 95%.

For indoor use only.

Chapter 7: Specifications and Characteristics
Trace Port Analyzer Environmental Characteristics

Troubleshooting the Emulation Module

Troubleshooting the Emulation Module

If you have problems with the emulation module, your first task is to determine the source of the problem. Problems may originate in any of the following places:

- The connection between the emulation module and your debugger
- The emulation module itself
- The connection between the emulation module and the Trace Port Analyzer
- The connection between the Trace Port Analyzer and the Target interface module
- The connection between the target interface module and the target system
- The target system

You can use several means to determine the source of the problem:

- The troubleshooting guide on the next page
- The status lights on the emulation probe or emulation module
- The emulator "performance verification" tests
- The Trace Port Analyzer "performance verification" tests
- The emulator's built-in "terminal interface" commands

Emulation Module Troubleshooting Guide

Common problems and what to do about them

Symptom	What to do	See also
Commands from debugger have no effect	Your debugger may not be configured properly. If this does not work, continue with the steps for the next symptom....	page 81
Emulation module built-in commands do not work	<p>1 Run the emulation module performance verification tests.</p> <p>2 If the performance verification tests pass, then there is an electrical problem with the connection to the target processor OR the target system may not have been designed according to "Designing a Target System."</p>	<p>page 97</p> <p>page 55, page 89</p>
"Slow or missing clock" message after a logic analyzer run	Check that the target system is running user code or is in reset. (This message can appear if the processor is in background mode.)	
Host computer reports LAN connection problems	Follow the checklist in the "If you have LAN problems" section.	page 93
Commands from the Run Control tool or debugger have no effect	Verify LAN communication.	page 37

Status Lights

Emulation Module Status Lights

The emulation module uses status lights to communicate various modes and error conditions.

The following table gives more information about the meaning of the power and target status lights.



- = LED is off
- = LED is on
- * = Not applicable (LED is off or on)

Power/Target Status Lights

Pwr/Target LEDs	Meaning
<input type="radio"/> Reset <input type="radio"/> Break <input type="radio"/> Run	No target system power, or emulation module is not connected to the target system
<input checked="" type="radio"/> Reset <input type="radio"/> Break <input type="radio"/> Run	Target system is in a reset state
<input type="radio"/> Reset <input checked="" type="radio"/> Break <input type="radio"/> Run	The target processor is executing in Debug Mode
<input type="radio"/> Reset <input type="radio"/> Break <input checked="" type="radio"/> Run	The target processor is executing user code
<input type="radio"/> Reset <input checked="" type="radio"/> Break <input checked="" type="radio"/> Run	Only boot firmware is good (other firmware has been corrupted)

Emulation Probe Status lights

The following illustration shows the status lights on both sides of the emulation probe and what they mean:

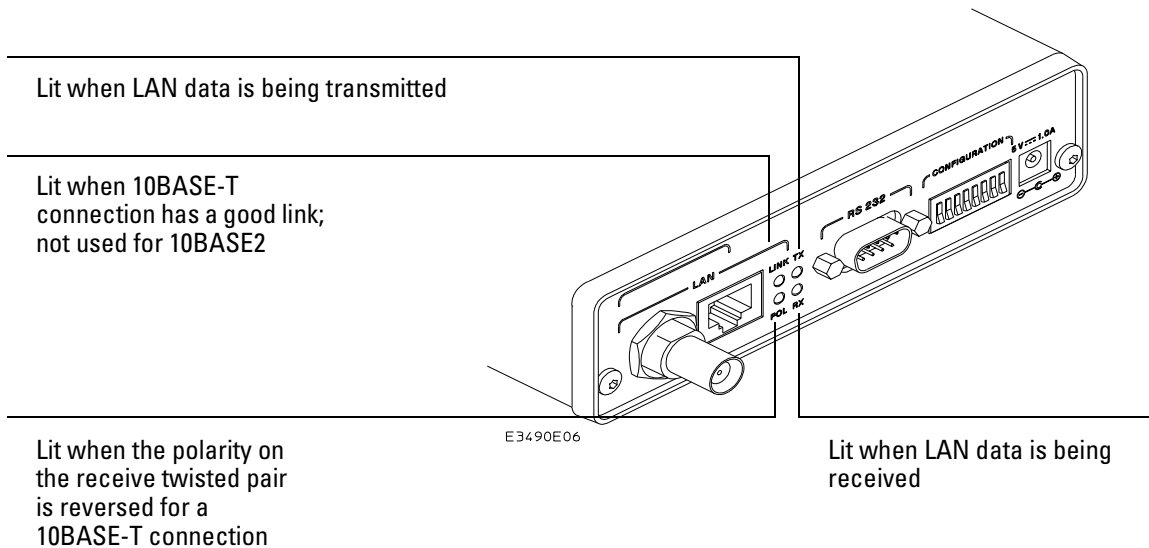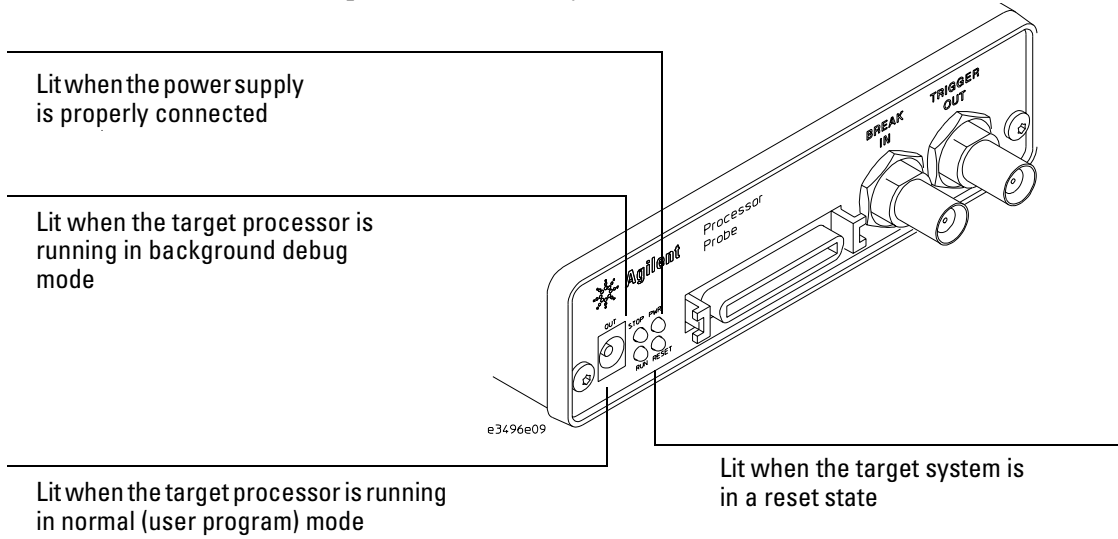

The emulation probe communicates various modes and error conditions via the status lights. The meanings of the status lights are shown on the previous page.

The following table gives more information about the meaning of the power and target status lights.

- = LED is off
- = LED is on
- * = Not applicable (LED is off or on)

Power/Target Status Lights

Pwr/Target LEDs	Meaning
○○ ○○	emulation probe is not connected to power supply
○● ○○	No target system power, or emulation probe is not connected to the target system
○● ○●	Target system is in a reset state
●● ●○	Only boot firmware is good (other firmware has been corrupted)
●● ○○	The target processor is executing in Debug Mode
○● ●○	The target processor is executing user code

Emulation Module Built-in Commands

The emulation module has some built-in "terminal interface" commands which you can use for troubleshooting. You can access the terminal interface using:

- A telnet (LAN) connection
- A "debugger command" window in your debugger
- A serial connection (see page 38)

To telnet to the emulation module

You can establish a telnet connection to the emulation module if:

- A host computer and the logic analysis system are both connected to a local-area network (LAN), and
- The host computer has the telnet program (often part of the operating system or an internet software package).

To establish a telnet connection:

- 1** Find out the port number of the emulation module.

The default port number of the first emulation module in an Agilent Technologies 16600A/700A series logic analysis system is 6472. The default port of a second module in an Agilent Technologies 16600A-series system is 6476. The default port numbers of a third and fourth module in an expansion frame are 6480 and 6484. These port numbers can be changed, but that is rarely necessary.

- 2** Find out the LAN address or LAN name of the logic analysis system.
- 3** Start the telnet program.

If the LAN name of the logic analysis system is "test2" and you have only one emulation module installed, the command might look like this:

```
telnet test2 6472
```

- 4** If you do not see a prompt, press the <Return> key a few times.

To exit from this telnet session, type <CTRL>D at the prompt.

To use the built-in commands

Here are a few commonly used built-in commands:

Useful built-in commands

b	Break -- go into the background monitor state
cf	Configuration -- read or write configuration options
help	Help -- display online help for built-in commands
init	Initialize -- init -c re-initializes everything in the emulation module except for the LAN software; init -p is the equivalent of cycling power (it will break LAN connections)
lan	configure LAN address
m	Memory -- read or write memory
reg	Register -- read or write a register
r	Run -- start running user code
rep	Repeat -- repeat a command or group of commands
rst	Reset -- reset the target processor (the emulation module will wait for you to press the target's RESET button)
s	Step -- do a low-level single step
ver	Version -- display the product number and firmware version of the emulation module

The prompt indicates the status of the emulation module:

Emulation module prompts

U	Running user program
M	Running in background monitor
p	No target power
R	Emulation reset
r	Target reset
?	Unknown state

Examples

To set register R0, then view R0 to verify that it was set, enter:

```
R>rst -m
M>reg r0=ffff
M>reg r0
reg R0=0000ffff
```

To break execution then step a single instruction, enter:

```
M>b
M>s
PC=xxxxxxxx
M>
```

To determine what firmware version is installed in the emulation module, enter:

```
M>ver
```

See Also

Use the help command for more information on these and other commands. Note that some of commands listed in the help screens are generic commands for Agilent Technologies emulators and may not be available for your product.

If you are writing your own debugger, contact Agilent Technologies for more information.

Problems with the LAN Interface (Emulation Probe Only)

If you cannot verify LAN communication

If you cannot verify connection using the procedure in "To verify LAN communication", or if the commands are not accepted by the emulation probe:

- Make sure that you have connected the emulation probe to the proper power source and that the power light is lit.
- Make sure that you wait for the power-on self test to complete before connecting.
- Make sure that the LAN cable is connected. Watch the LAN LED's to see whether the emulation probe is seeing LAN activity. Refer to your LAN documentation for testing connectivity.
- Make sure that only one of the LAN ports is connected.
- Make sure the emulation probe communication configuration switches are set correctly. Unplug the emulation probe power cord, then plug it in again to make sure the switch settings are read correctly by the emulation probe.
- Check that the Run Control Tool or debugger was configured with the correct LAN address. If the emulation probe is on a different subnet than the host computer, check that the gateway address is correct.
- Make sure that the emulation probe's IP address is set up correctly. Use the RS-232 port to verify this that the IP address is set up correctly. When you are connected to the RS-232 port, run performance verification on the emulation probe's LAN interface with the "pv" command.
- It's also possible for there to be a problem with the emulation probe firmware while the LAN interface is still up and running. In this case, you must reboot the emulation probe by disconnecting power to the emulation probe and reconnecting it again.
- Use a serial connection to run the LAN performance verification tests (see page 97).

If you have LAN connection problems

- ❑ If the emulation probe does not accept commands from the logic analysis system:
 1. Check that switch S1 is "0" (attached to LAN, not RS-232).
 2. Check that switch S5 is in the correct position for your LAN interface (either 10BASE2 or 10BASE-T).(Remember: if you change any switch settings, the changes do not take effect until you cycle power.)
- ❑ If the emulation probe still does not respond, you need to verify the IP address and gateway mask of the emulation probe. To do this, connect the emulation probe to a terminal or terminal emulator (see page 38), change the switch settings so it is connected to RS-232, and enter the "lan" command. The output looks something like this:

```
lan -i 15.5.24.116
lan -g 15.5.23.1
lan -p 6470
Ethernet Address : 08000909BAC1
```

"lan -i" shows the internet address is 15.5.24.116 in this case. If the Internet address (IP) is not what you expect, you can change it with the 'lan -i <new IP>' command.

"lan -g" shows the gateway address. Make sure it is the address of your gateway if you are connecting from another subnet, or 0.0.0.0 if you are connecting from the local subnet.

"lan -p" shows the port is 6470. If the port is not 6470, you must change it with the "lan -p 6470" command (unless you have deliberately set the port number to a different value because of a conflict).

If the "POL" LED is lit

The "POL" LED indicates that the polarity is reversed on the receive pair if you are using a 10BASE-T connection. The emulation probe should still work properly in this situation, but other LAN devices may not work.

If it takes a long time to connect to the network

- ❑ Check the subnet masks on the other LAN devices connected to your network. All of the devices should be configured to use the same subnet mask.

Subnet mask error messages do not indicate a major problem. You can continue using the emulation probe.

The emulation probe automatically sets its subnet mask based on the first subnet mask it detects on the network. If it then detects other subnet masks, it will generate error messages.

If there are many subnet masks in use on the local subnet, the emulation probe may take a very long time to connect to the network after it is turned on.

To "clean up" the network, connect a terminal to the emulation probe. You can then see error messages which will help you identify which devices on the network are using the wrong subnet masks.

Problems with the Serial Interface (Emulation Probe Only)

If you cannot verify RS-232 communication

If the emulation probe prompt does not appear in the terminal emulator window:

- Make sure that you have connected the emulation probe to the proper power source and that the power light is lit.
- Make sure that you have properly configured the data communications switches on the emulation probe and the data communications parameters on the host computer. You should also verify that you are using the correct cable.

The most common type of data communications configuration problem involves the configuration of the emulation probe as a DTE device instead of as a DCE device. If you are using the wrong type of cable, no prompt will be displayed.

A cable with one-to-one connections will work with a PC or a Hewlett-Packard Series 700 workstation.

If you have RS-232 connection problems with the MS Windows Terminal program

- Remember that Windows 3.1 only allows two active RS-232 connections at a time. To be warned when you violate this restriction, choose Always Warn in the Device Contention group box under 386 Enhanced in the Control Panel.
- Use the "Terminal" program (usually found in the Accessories windows program group) and set up the "Communications..." settings as follows:

Baud Rate: 9600 (or whatever you have chosen for the emulator)

Data Bits: 8

Parity: None

Flow Control: hardware

Stop Bits: 1

When you are connected, hit the Enter key. You should get a prompt back. If nothing echos back, check the switch settings on the emulation probe.

- ❑ If the switches are in the correct position and you still do not get a prompt when you hit return, try turning OFF the power to the emulation probe and turning it ON again.
- ❑ If you still don't get a prompt, make sure the RS-232 cable is connected to the correct port on your PC, and that the cable is appropriate for connecting the PC to a DCE device.

With certain RS-232 cards, connecting to an RS-232 port where the emulation probe is turned OFF (or is not connected) will hang the PC. The only way to get control back is to reboot the PC. Therefore, we recommend that you always turn ON the emulation probe before attempting to connect via RS-232.

Problems with the Target System

This section describes how to determine whether your target system is causing problems with the operation of the emulation module.

What to check first

- 1 Try some basic built-in commands using the Command Line window or a telnet connection:

```
U>rst  
R>
```

This should reset the target and display a "R>" prompt.

```
R>b  
M>
```

This should stop the target and display an "M>" prompt.

```
M>reg r1  
reg r1=00000000  
M>
```

This should read the value of the r1 register (the value will probably be different on your target system).

```
M>m 0..  
00000000 7c3043a6 7c2802a6 7c3143a6 4bf04111  
00000010 00000000 00000000 00000000 00000000  
00000020 00000000 00000000 00000000 00000000  
00000030 00000000 00000000 00000000 00000000  
00000040 00000000 00000000 00000000 00000000  
00000050 00000000 00000000 00000000 00000000  
00000060 00000000 00000000 00000000 00000000  
00000070 00000000 00000000 00000000 00000000  
M>
```

This should display memory values starting at address 0.

```
M>s
```

This should execute one instruction at the current program counter.

If any of these commands don't work, there may be a problem with the design of your target system, a problem with the revision of the emulation you are using, or a problem with the configuration of the emulation module. The following steps will help you identify the problem.

- 2 Check that the emulation module firmware matches your processor. To do this, enter:

M>ver

See Also

Page 81 for information on entering built-in commands.

To interpret the initial prompt

The initial prompt can be used to diagnose several common problems. To get the most information from the prompt, follow this procedure:

- 1 Connect the emulation module to your target system.
- 2 Set the default configuration settings. Enter:

M>init -c

You can enter this command at any prompt. The emulation module will respond with the same information as printed by the "ver" command.

If the response is "!ERROR 905! Driver firmware is incompatible with ID of attached device"

Make sure the target interface module is connected to the cable of the emulation module, then try the "init -c" command again.

If the initial prompt is "p>"

Check pin 3 on header.

If the initial prompt is "M>"

The processor entered debug mode without the help of the emulation module. Is another debugger connected?

If the initial prompt is "U>"

The emulation module is scanning the instruction register correctly. Now you can do some more tests:

- 4 Enter the reset command:

```
U>rst  
R>
```

The "R>" prompt is a good response that indicates SRESET and HRESET are working.

Problems with the LAN Interface

If LAN communication does not work

If you cannot verify connection using the procedure in "To verify LAN communication", or if the commands are not accepted by the emulation module:

- Make sure that you wait for the power-on self test to complete before connecting.
- Make sure that the LAN cable is connected. Watch the LAN LED's on the back of the logic analysis system to see whether the system is seeing LAN activity. Refer to your LAN documentation for testing connectivity.
- Check that the host computer or debugger was configured with the correct LAN address. If the logic analysis system is on a different subnet than the host computer, check that the gateway address is correct.
- Make sure that the logic analysis system's IP address is set up correctly.

If it takes a long time to connect to the network

- ❑ Check the subnet masks on the other LAN devices connected to your network. All of the devices should be configured to use the same subnet mask.

Subnet mask error messages do not indicate a major problem. You can continue using the emulation module.

The subnet mask is set in the logic analysis system's System Admin window. If it then detects other subnet masks, it will generate error messages.

If there are many subnet masks in use on the local subnet, the logic analysis system may take a very long time to connect to the network after it is turned on.

Problems with the Emulation Probe

To run the power up self test

- 1 Unplug the emulation probe, then plug it in.
- 2 Watch the status lights. They should show the following pattern:
 - = LED is off
 - = LED is on
 - * = Not applicable (LED is off or on)

Normal sequence during power up self test

	Pwr/Target LEDs	Meaning
1	○● ○○	Initial power up, system reset
2	○● ○○	XILINX array initialized successfully
3	○● ●○	XILINX array tested successfully
4	●● ○○	BOOT ROM space tested successfully
5	○● ●○	GENERIC ROM space tested successfully
6	●● ○○	DRIVER ROM space tested successfully
7	○● ●○	RESERVED ROM space tested successfully
8	●● ○○	RAM tested successfully
9	○● ●○	LAN internal feedback tested successfully
10	○● ○○	Boundary scan master (BSM) test begun
11	●● ○●	BSM test completed, start system, load drivers, initialize LAN

If the power up self test fails, the RESET LED will flash the number of the test, then stay lit.

If any of the LEDs fail to change, or all of them remain on, there is a system failure.

Following power up, the LEDs will enter one of the following states:

- No target system power, or emulation probe is not connected to the target system, or
○○
- Target system is in a reset state
○○
- Only the boot ROM was used; other firmware in the Flash EPROM has been corrupted
●○

Starting a user interface will change the pattern to the one requested by the interface.

If the power up self tests fail, try the following:

- Check and reset the LAN address as shown in the "Connecting to a Host Computer" chapter. LAN powerup failures will occur if the emulation probe does not have a valid Link Level Address and IP Address.
- Disconnect all external connections, including the LAN, serial (RS-232), and BNC Break and Trigger cables, then cycle power.
- To ensure that the firmware is working as it should, reprogram the firmware, then cycle power.


To execute the built-in performance verification test (emulation probe only)

In addition to the powerup tests, there are several additional performance verification (PV) tests available.

Some of these tests can be performed through the logic analysis system. The LAN tests can only be executed through the RS-232 port.

To perform the PV tests through the logic analysis system

- 1 End any Emulation Control Interface sessions.
- 2 Disconnect the 50-pin cable from the emulation probe, and plug the loopback test board into the emulation probe.

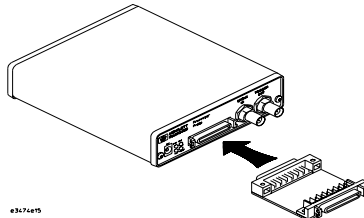

- 3 Connect a BNC cable from the “Break In” connector to the “Trigger Out” connector on the emulation probe.
- 4 From the emulation probe icon menu, open the Performance Verification window.
- 5 Enter the LAN address of the emulation probe.
- 6 Select the number of iterations to perform.
- 7 Click **Start PV**.

The results will appear on screen.

Additional PV Tests

The LAN tests can only be executed through the RS-232 port. The remainder of this section assumes that the tests are being run from a terminal emulator connected to the RS-232 port.

For the BREAK IN, TRIGGER OUT BNC FEEDBACK TEST, connect a coaxial cable between BREAK IN and TRIGGER OUT.

For the TARGET PROBE FEEDBACK TEST, connect the self-test board (Agilent part number E3496-66502).

- 1 Set all of the switches to OPEN.

This is standard RS-232 at 9600 baud which can be connected directly to a 9 pin RS-232 interface that conforms to the IBM PC-AT 9 pin standard.

- 2 Use a terminal emulator to connect to the emulation probe.
- 3 Enter the **pv** command.

Options available for the "pv" are explained in the help screen displayed by typing "help pv" or "? pv" at the prompt.

Examples:

To execute both tests one time:

```
pv 1
```

To execute test 2 with maximum debug output repeatedly until a ^C is entered:

```
pv -t2 -v9 0
```

To execute tests 3, 4, and 5 only for 2 cycles:

```
pv -t3-5 2
```

On a good system, when the feedback connector is plugged into the target connector, the RESET LED will light and the BKG and USER LEDs will be out.

The results on a good system, with the BNC's connected, and with the self-test board plugged in, are as follows:

```
R>pv 1
```

```
Testing: E3499A Series Emulation System
```

```
Test # 1: Powerup PV Results           Passed!
Test # 2: LAN 10Base2 Feedback Test     Passed!
Test # 3: LAN 10BaseT Feedback Test     Passed!
Test # 4: Break In and Trigger Out BNC Feedback Test  Passed!
Test # 5: Target Probe Feedback Test     Passed!
Test # 6: Boundary Scan Master Test     Passed!
Test # 7: I2C                           Passed!
```

```
PASSED Number of tests: 1      Number of failures: 0
```

Copyright (c) Agilent Technologies 1987

All Rights Reserved. Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under copyright laws.

```
E3499A Series Emulation System
```

```
Version: A.05.05 18Nov96 07:47 Proto
```

```
Location: Generics
```

There are some things you can do if a failure is found on one of these tests. Details of Failure can be obtained through using a verbose level of 2 or more.

If the particular failure you see is not listed below, contact Agilent Technologies for assistance.

TEST 2: LAN 10BASE2 Feedback Test failed

For LAN 10BASE2 test, the following is an example of a failure which is *not* caused by a broken emulation probe.

R>pv -t2 -v2 1

Testing: E3499A Series Emulation System

Test # 2: LAN 10Base2 Feedback Test failed!

FAILED - no lan connection (LAN probably not terminated)

FAILED Number of tests: 1 Number of failures: 1

Check to see that the port under test has a good cable connected to it and that the cable is properly terminated with a 50 ohm terminator on each end of the overall cable.

R>pv -t2 -v2 1

Testing: E3499A Series Emulation System

Test # 2: LAN 10Base2 Feedback Test failed!

FAILED due to excessive collisions

FAILED Number of tests: 1 Number of failures: 1

The most common cause of this problem is poor termination of the cable or failure to remove the port under test from the LAN before performing the test. Check to see that the terminators are good (50 Ohms) and that you are isolated from any traffic on a system LAN.

R>pv -t2 -v2 1

Testing: E3499A Series Emulation System

Test # 2: LAN 10Base2 Feedback Test failed!

FAILED - invalid Ethernet address in EEPROM

FAILED Number of tests: 1 Number of failures: 1

First check to see that a correct LLA and IP address have been set in the virtual EEPROM through the "lan" command. If the "lan" command shows bad information for the LLA and IP, then try to set them to correct values. If you are unable to set them to correct values, there is a failure in the FLASH ROM which requires service from Agilent Technologies.

Test 3: 10BaseT Feedback Test failed

R>pv -t3 -v2 1

Testing: E3499A Series Emulation System
Test # 3: LAN 10BaseT Feedback Test passed!
PASSED Number of tests: 1 Number of failures: 0

In addition to the internal checks performed in Test 2, this test also checks for shorts on the cable connected to the network. If this test fails, disconnect the cable and run the test again. If it then passes, the cable is faulty. If it still fails, it requires service from Agilent Technologies.

If the emulation probe passes this "pv" test, additional testing can be performed through exercising the connection to the network. To run this test, set configuration switch 1 and switch 5 to OPEN, all other configuration switches CLOSED (this enables LAN using 10BaseT). Cycle power and wait for 15 to 30 seconds. Then "ping" the emulaiton probe from your host computer or PC. See the LAN documentation for your host computer for the location and action of the "ping" utility. If the emulaiton probe fails to respond to the "ping" request, verify that the lan parameters (IP address and gateway address) are set correctly and that your host computer recognizes the IP address of the emulation probe. If all else is good, then failure to respond to ping indicates a faulty emulation probe.

E3499A TEST 4: Break In and Trigger Out BNC Feedback Test

R>pv -t4 -v2 1

Testing: E3499A Series Emulation System
Test # 4: Break In and Trigger Out BNC Feedback Test failed!
Break In not receiving Break Out HIGH
FAILED Number of tests: 1 Number of failures: 1

Before returning to Agilent Technologies, check to ensure that you have connected a good Coaxial cable between the two BNCs. If the cable is good, the emulation probe is bad.

TEST 5: Target Probe Feedback Test

A verbose output on this test can be extensive. For example, the following is the output of this test if you forget to plug in the self-test board.

```
p>pv -t5 -v2 1
```

```
Testing: E3499A Series Emulation System
Test # 5: Target Probe Feedback Test          failed!
Bad 20 Pin Status Read when unconnected = 0x7fb7
    Expected Value = 0xffb7
Bad 20 Pin Status Read when connected= 7fb7
    Expected Value = 0x7fb7
Output 19 Low not received on Input 11
Output 11 Low not received on Input 19
Output 13 Low not received on Input 1
Output 12 High not received on Input 6
Output 12 and Input 6 not pulled high on release
Output 8 Low not received on Input 10
Output 7 Low not received on Input 20
Output 4 Low not received on Input 14
Output 2 Low not received on Input 18
FAILED Number of tests: 1      Number of failures: 1
```


If the you get a verbose output like this, check to make sure that the self test board was connected properly.

Problems with the Emulation Module

Occasionally you may suspect a hardware problem with the emulation module or target interface module. The procedures in this section describe how to test the hardware, and if a problem is found, how to repair or replace the broken component.

To run the built-in performance verification test using the logic analysis system (emulation module only)

- 1 End any Emulation Control Interface or debugger sessions.
- 2 Disconnect the 50-pin cable from the emulation module, and plug the loopback test board (Agilent part number E3496-66502) into the emulation module.

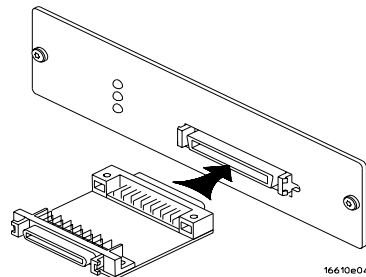

- 3 In the system window, click the emulation module and select **Performance Verification**.
- 4 Click **Start PV**.
The results will appear on screen.

To run complete performance verification tests using a telnet connection (emulation module only)

- 1 Disconnect the 50-pin cable from the emulation module, and plug the loopback test board (Agilent part number E3496-66502) directly into the emulation module. Do not plug anything into the other end of the loopback test board.

On a good system, the RESET LED will light and the BKG and USER LEDs will be out.

- 2 telnet to the emulation module.
- 3 Enter the **pv 1** command.

See Also

Options available for the "pv" command are explained in the help screen displayed by typing "help pv" or "? pv" at the prompt. Note, however, that some of the options listed may not apply to your emulation module.

Examples:

If you are using a UNIX system, to telnet to a logic analysis system named "mylogic", enter:

```
telnet mylogic 6472
```

Here are some examples of ways to use the **pv** command.

To execute both tests one time:

```
pv 1
```

To execute test 2 with maximum debug output repeatedly until a ^C is entered:

```
pv -t2 -v9 0
```

To execute tests 3, 4, and 5 only for 2 cycles:

```
pv -t3-5 2
```

The results on a good system with the loopback test board connected, are as follows:

```
M>pv 1
```

```
Testing: E3499C Series Emulation System
Test 1: Powerup PV Results           Passed!
Test 2: Target Probe Feedback Test   Passed!
Test 3: Boundary Scan Master Test    Passed!
Test 4: I2C Test                     Passed!
Test 5: Data Lines Test              Passed!
PASSED Number of tests: 1           Number of failures: 0
```

Copyright (c) Agilent Technologies 1987
All Rights Reserved. Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under copyright laws.


E3499C Series Emulation System
Version: A.07.51 17Dec97
Location: Generics

E3497A Motorola MPC800 Embedded PowerPC Emulator
Version: A.01.02 18Dec97
M>

Problem with the Trace Port Analyzer and TIM

To perform the TIM and Trace Port Analyzer PV tests with an emulation probe/module

- 1 End any Emulation Control Interface or debugger sessions.
- 2 Disconnect the 20-pin cable from a target system, and plug the target end of 20-pin cable into loop-back connector on a TIM.

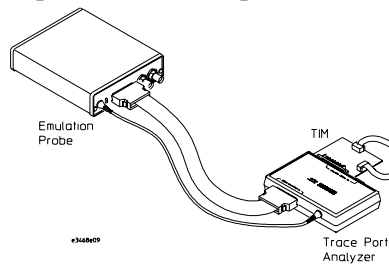

- 3 Telnnet to the emulation probe/module.
- 4 Enter **pv 1** command.

The result will appear on screen as below.

```
Testing: E3499B Series Emulation System
Test 1: Powerup PV Results           Passed!
Test 2: LAN 10Base2 Feedback Test     Not Executed!
Test 3: LAN 10BaseT Feedback Test     Not Executed!
Test 4: Break In and Trigger Out BNC Feedback Test Passed!
Test 5: Target Probe Feedback Test    Not Executed!
Test 6: Boundary Scan Master Test     Not Executed!
Test 7: I2C Test                     Not Executed!
Test 8: Data Lines Test               Passed!
Testing: E3468A Toshiba TX19/39 Series Emulator
Test 1: E3468 TIM/TP Test             Passed!
PASSED Number of tests: 1      Number of failures: 0
```

Copyright (c) Agilent Technologies 1987
All Rights Reserved. Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under copyright laws.


Chapter 8: Troubleshooting the Emulation Module
Problem with the Trace Port Analyzer and TIM

E3499B Series Emulation System
Version: A.07.07 06Jul98 12:56 Proto
Location: Generics

E3468A Toshiba TX19/39 Series Emulator
Version: A.01.00 00Jan00

To perform the TIM only PV tests with an emulation probe/module

- 1 End any Emulation Control Interface or debugger sessions.
- 2 Disconnect the trace port analyzer, and connect a TIM to 50-pin cable directly.
- 3 Disconnect the TIM board from the trace port analyzer, and plug the loop-back board into the trace port analyzer.

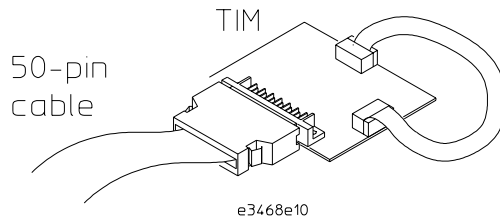

- 4 Telnet to the emulation probe/module.
- 5 Enter **pv 1** command.

The result will appear on screen as below.

```
Testing: E3499B Series Emulation System
Test 1: Powerup PV Results           Passed!
Test 2: LAN 10Base2 Feedback Test    Not Executed!
Test 3: LAN 10BaseT Feedback Test    Not Executed!
Test 4: Break In and Trigger Out BNC Feedback Test Passed!
Test 5: Target Probe Feedback Test    Not Executed!
Test 6: Boundary Scan Master Test    Not Executed!
Test 7: I2C Test                     Not Executed!
Test 8: Data Lines Test              Passed!
Testing: E3468A Toshiba TX19/39 Series Emulator
Test 1: E3468 TIM Test               Passed!
PASSED Number of tests: 1      Number of failures: 0
```

Copyright (c) Agilent Technologies 1987
All Rights Reserved. Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under copyright laws.

E3499B Series Emulation System
Version: A.07.07 06Jul98 12:56 Proto
Location: Generics

E3468A Toshiba TX19/39 Series Emulator
Version: A.01.00 00Jan00

If a performance verification test fails

- Details of the failure can be obtained through using a -v option ("verbose" level) of 2 or more.
- Check that the loopback test board is connected.
- If the problem persists, contact Agilent Technologies for assistance.

Returning Parts to Agilent Technologies for Service

The repair strategy for this emulation solution is board replacement.

Exchange assemblies are available when a repairable assembly is returned to Agilent Technologies. These assemblies have been set up on the "Exchange Assembly" program. This lets you exchange a faulty assembly with one that has been repaired, calibrated, and performance verified by the factory. The cost is significantly less than that of a new assembly.

To return a part to Agilent Technologies

- 1 Follow the procedures in this chapter to make sure that the problem is caused by a hardware failure, not by configuration or cabling problems.
- 2 In the U.S., call 1-800-403-0801. Outside the U.S., call your nearest Agilent Technologies sales office. Ask them for the address of the nearest Agilent Technologies service center.
- 3 Package the part and send it to the Agilent Technologies service center.
Keep any parts which you know are working. For example, if only the target interface module is broken, keep the emulation module and cables.
- 4 When the part has been replaced, it will be sent back to you.
The unit returned to you will have the same serial number as the unit you sent to Agilent Technologies.

The Agilent Technologies service center can also troubleshoot the hardware and replace the failed part. To do this, send your entire measurement system to the service center, including the logic analysis system, target interface module, and cables.

In some parts of the world, on-site repair service is available. Ask an Agilent Technologies sales or service representative for details.

To obtain replacement parts

The following table lists some parts that may be replaced if they are damaged or lost. The part numbers are subject to change. Contact your nearest Agilent Technologies Sales Office for further information.

Part numbers

Exchange Assemblies

Part Number	Description
16600-69515	Emulation module
E3468-66401	Programmed emulation probe assembly

Replacement Assemblies

Part Number	Description
E3492-61601	20-pin target cable
E3496-61601	50-pin cable
E3496-66502	Loopback test board
E3468-66501	Target Interface Module
16700-61608	Expansion cable for emulation module
0950-3043	Power supply for emulation probe
E5890-64301	Trace Port Analyzer
E5890-66502	Trace Port Analyzer loopback test board

Cleaning the Instrument

If the instrument requires cleaning:

- 1 Remove power from the instrument.
- 2 Clean the instrument with a mild detergent and water.
- 3 Make sure that the instrument is completely dry before reconnecting it to a power source.

Glossary

Analysis Probe

A probing solution connected to the target microprocessor. It provides an interface between the signals of the target microprocessor and the inputs of the logic analyzer. Formerly called a "preprocessor."

Elastomeric Probe Adapter

A connector that is fastened on top of a target microprocessor using a retainer and knurled nut. The conductive elastomer on the bottom of the probe adapter makes contact with pins of the target microprocessor and delivers their signals to connection points on top of the probe adapter.

Emulation Module

An emulation module is installed within the mainframe of a logic analyzer. It provides run control within an emulation and analysis test setup. See Emulation Probe.

Emulation Probe

An emulation probe is a standalone instrument connected to the mainframe of a logic analyzer. It provides run control within an emulation and analysis test setup. Formerly called a

"processor probe" or "software probe." See Emulation Module.

Extender

A part whose only function is to provide connections from one location to another. One or more extenders might be stacked to raise a probe above a target microprocessor to avoid mechanical contact with other components installed close to the target microprocessor. Sometimes called a "connector board."

Flexible Adapter

Two connection devices coupled with a flexible cable. Used for connecting probing hardware on the target microprocessor to the analysis probe.

General-Purpose Flexible Adapter

A cable assembly that connects the signals from an elastomeric probe adapter to an analysis probe. Normally, a male-to-male header or transition board makes the connections from the general-purpose flexible adapter to the analysis probe.

High-Density Adapter Cable

A cable assembly that delivers signals from an analysis probe hardware

interface to the logic analyzer pod cables. A high-density adapter cable has a single Mictor connector that is installed into the analysis probe, and two cables that are connected to corresponding odd and even logic analyzer pod cables.

High-Density Termination Adapter Cable

Same as a High-Density Adapter Cable, except it has a termination in the Mictor connector.

Jumper

Moveable direct electrical connection between two points.

Mainframe Logic Analyzer

A logic analyzer that resides on one or more board assemblies installed in an Agilent Technologies 16500, Agilent Technologies 1660x, or Agilent Technologies 16600A/700A-series mainframe.

Male-to-male Header

A board assembly that makes point-to-point connections between the female pins of a flexible adapter or transition board and the female pins of an analysis probe.

Preprocessor

See Analysis Probe.

Preprocessor Interface

See Analysis Probe.

Probe adapter

See Elastomeric Probe Adapter.

Processor Probe

See Emulation Probe.

Prototype Analyzer

The Agilent Technologies 16505A prototype analyzer acts as an analysis and display processor for the Agilent Technologies 16500B/C logic analysis system. It provides a windowed interface and powerful analysis capabilities. Replaced by Agilent Technologies 16600A/700A-series logic analysis systems.

Run Control Probe

See Emulation Probe and Emulation Module.

Setup Assistant

A software program that guides a user through the process of connecting and configuring a logic analyzer to make measurements on a specific microprocessor.

Shunt Connector.

See Jumper.

Software Probe

See Emulation Probe.

Solution

Agilent Technologies' term for a set of tools for debugging your target system. A solution includes probing, inverse assembly, the Agilent Technol-

ologies B4620B Source Correlation Tool Set, and possibly an emulation module.

Stand-alone Logic Analyzer

A standalone logic analyzer has a predefined set of hardware components which provide a specific set of capabilities. It is designed to perform logic analysis. A standalone logic analyzer differs from a mainframe logic analyzer in that it does not offer card slots for installation of additional capabilities, and its specifications are not modified based upon selection from a set of optional hardware boards that might be installed within its frame.

Target Control Port

An 8-bit, TTL port on a logic analysis system that you can use to send signals to your target system. It does not function like a pattern generator or emulation module, but more like a remote control for the target's switches.

Target Interface Module

A small circuit board which connects the 50-pin cable from an emulation module or emulation probe to signals from the debug port on a target system.

TIM

See Target Interface Module.

Trace Port Analyzer

A small logic analyzer which was specialized for PC-Trace function dedicated in Tx19/39 series processors.

Trigger Specification

A set of conditions that must be true before the instrument triggers. See the printed or online documentation for your logic analyzer for details.

Transition Board

A board assembly that obtains signals connected to one side and rearranges them in a different order for delivery at the other side of the board.

1/4-Flexible Adapter

An adapter that obtains one-quarter of the signals from an elastomeric probe adapter (one side of a target microprocessor) and makes them available for probing.

Index

A

- address, IP
 - See* IP address
- altitude specifications, 73
- analysis probe
 - connecting to, 61
 - definition, 113
 - equipment required, 16
 - equipment supplied, 14
 - overview, 2
 - processors supported, 4
 - product numbers, 4

B

- BDM port
 - See* debug port
- BKG light, 98, 103
- BNC
 - LAN, 29
- BNC, LAN, 71
- BOOTP, 34
- built-in commands
 - LAN configuration, 31
 - list of commands, 81–83

C

- cable
 - LAN, 36
 - power, 18
 - serial, 39
- cables
 - emulator, 59
 - replacing, 110
- CD-ROM, installing software from, 52
- checklist, setup, 13
- cleaning, 111
- clocks
 - specifications, 71
- configuration
 - flowchart, 13
- configuration files
 - installing, 49, 51–52
- connection
 - emulation module, 43–44, 53–54
 - host workstation, 27–41
 - problems, LAN, 85, 93
 - problems, RS-232, 87
- connector

- 10BASE2, 29–37, 71
- 10BASE-T, 29–37, 71
- serial, 71

connector board, 113

D

- data communications
 - specifications, 71
- DCE or DTE selection and RS-232 cable, 87
- debug port
 - connecting to, 59
- debuggers
 - writing, 83
- development port
 - See* debug port
- directories
 - software installation, 52
- driver firmware error, 91

E

- elastomeric probe adapter
 - definition, 113
- emulation module
 - 16600 installation, 47
 - 16700A installation, 45
 - connecting, 44–48, 54, 58–61
 - definition, 113
 - description of, 3
 - product numbers, 4
 - target system design, 55–57
- emulation probe
 - definition, 113
- emulation solution
 - See* solution
- equipment required
 - emulation migration, 25
 - emulation module, 20
 - trace port analyzer, 22
- equipment supplied
 - analysis probe, 14
 - emulation migration, 24–25
 - emulation module, 19–20
 - ordering information, 4
 - overview, 4
 - trace port analyzer, 21–22
- ethernet address, 31
- extender, 113

F

- files
 - loading vs. installing, 50
- firmware, updating, 64
- flash EPROM, 64
- flexible adapter
 - definition, 113
- flowchart, setup, 13
- full solution, 3

G

- gateway address, 32, 85
- general-purpose flexible adapter
 - definition, 113

H

- high-density adapter cable
 - definition, 113
- high-density termination adapter cable
 - definition, 114
- host computer
 - connecting to, 27–41

I

- IEEE 802.3, 29–37
- information sources, 26
- init command, 91
- installation, software, 49, 51–52
- internet address
 - See* IP address
- IP address, 29–31, 84–85

J

- jumper, definition, 114

L

- LAN
 - problems, 93–94
- lan command, 31
- LAN connection problems, 85, 99–100
- LAN interface, 29–37
- LAN parameters, configuring
 - BOOTP, 34
 - methods, 29
 - terminal interface, 31
- lights
 - See* status lights

Index

-
- link beat, 36
 - link level address, 31, 34
 - LINK light, 79
 - loading configurations, vs. installing, 49, 51–52
 - M**
 - mainframe logic analyzer
 - definition, 114
 - male-to-male header
 - definition, 114
 - mask, subnet, 86, 94
 - MAU, 29, 71
 - microprocessors supported, 4
 - P**
 - PC
 - connecting to, 27–41
 - performance verification test, 97, 102
 - ping command, 85
 - POL light, 79, 86
 - port number, 32
 - port number, emulation module, 81
 - power cord, 16–18
 - power failure during firmware update, 65
 - power on/off sequence, 18
 - power up self test, 95
 - preprocessor
 - See* analysis probe
 - prgflash, 64
 - probe, testing, 101
 - problems
 - emulation module, 75–111
 - processor support package, 52
 - processors supported, 4
 - prompts, 83
 - list of, 83
 - troubleshooting, 91
 - prototype analyzer
 - definition, 114
 - PV
 - See* performance verification test
 - R**
 - references, 26
 - register commands, 89
 - repair
 - emulation module, 109–111
 - requirements
 - target system, 55–57
 - RESET
 - light, 78
 - signal, 55
 - RESET light, 79
 - RS-232
 - See* serial connection
 - run control tool
 - See* emulation control interface
 - S**
 - self test, 95
 - serial connection
 - DCE or DTE selection, 87
 - number of connections, 87
 - problems, 87
 - setting up, 38–41
 - verifying, 41
 - service ports, TCP, 32
 - service, how to obtain, 109
 - setup assistant
 - definition, 114
 - setup checklist, 13
 - slow clock, 77
 - software
 - installing, 49
 - list of installed, 51
 - software probe
 - See* emulation module
 - See* emulation probe
 - solution
 - at a glance, 2
 - definition, 114
 - solutions
 - description of, 2
 - product numbers, 4
 - specifications
 - altitude, 73
 - clock, 71
 - data communications, 71
 - temperature, 73
 - trigger in/out, 71
 - StarLAN, 29, 36
 - status lights, 78–80, 95
 - subnet mask, 29, 85–86, 94
 - switches
 - bootp, 35
 - LAN configuration, 31, 36
 - serial configuration, 39
 - T**
 - target control port, 115
 - target interface module (TIM)
 - connecting, 59
 - definition, 115
 - target system
 - connecting to, 44–48, 54
 - problems with, 89–92
 - requirements for emulation, 55–57
 - telnet, 37, 81, 84
 - temperature specifications, 73
 - terminal (MS Windows program), 87
 - terminal interface, 37
 - LAN parameters, setting, 31
 - See also* built-in commands
 - tests, emulation module, 102–108
 - ThinLAN, 29, 71
 - trace port analyzer
 - definition, 115
 - product numbers, 4
 - transition board
 - definition, 115
 - trigger
 - in/out specifications, 71
 - troubleshooting, 77
 - emulation module, 75–111
 - turning on power, 18
 - TX light, 79
 - U**
 - update, firmware, 64
 - USER light, 78–79
 - W**
 - web sites
 - logic analyzers, 26
 - workstation
 - connecting to, 27–41
-

DECLARATION OF CONFORMITY

according to ISO/IEC Guide 22 and EN 45014

Manufacturer's Name: Agilent Technologies Japan, Ltd.
Manufacturer's Address: 1-3-2, Murotani, Nishi-Ku, Kobe-shi, Hyogo, 651-22 Japan

declares, that the product

Product Name: Emulation Probe
Model Number(s): Agilent Technologies E3468A
Product Option(s): This declaration covers all options of the above product.

conforms to the following Product Specifications:

Safety: EN 61010-1:1993 / IEC 1010-1:1990+A1
EMC: EN 55011:1991 / CISPR 11:1990 - Group 1 Class A
EN 61000-3-2:1995 / IEC 1000-3-2:1995
EN 61000-3-3:1995 / IEC 1000-3-3:1994
EN 50082-1:1992
IEC 801-2:1991 - 4 kV CD, 8 kV AD
IEC 801-3:1984 - 3 V/m, 1 kHz 80% AM, 27 MHz - 1 GHz
IEC 801-4:1988 - 0.5 kV Signal Lines, 1 kV Power Lines

Supplementary Information:

The product herewith complies with the requirements of the EMC Directive 89/336/EEC and the Low Voltage Directive 73/23/EEC and carries the CE marking accordingly.

This product was tested in a typical configuration.

Kobe, September 9, 1998


Yukihiko Ota / Quality Manager

European Contact: Your local Agilent Technologies Sales and Service Office or Agilent Technologies GmbH, Department ZQ / Standards Europe, Herrenberger Strasse 130, D-71034 Böblingen Germany (FAX: +49-7031-14-3143)

Product Regulations

Safety IEC 1010-1:1990+A1 / EN 61010-1:1993
CSA-C22.2 No. 1010.1:1993

EMC This Product meets the requirement of the European Communities (EC) EMC Directive 89/336/EEC.



ISM 1-A

Emissions EN55011/CISPR 11 (ISM, Group 1, Class A equipment)
EN61000-3-2 / IEC61000-3-2
EN61000-3-3 / IEC61000-3-3

Immunity EN50082-1 Code¹

IEC 801-2 (ESD) 4kV CD, 8kV AD	1
IEC 801-3 (Rad.) 3 V/m	1
IEC 801-4 (EFT) 0.5 kV, 1kV	

¹Performance Codes:

1 PASS - Normal operation, no effect.

2 PASS - Temporary degradation, self recoverable.

3 PASS - Temporary degradation, operator intervention required.

4 FAIL - Not recoverable, component damage.

Sound Pressure Level N/A

DECLARATION OF CONFORMITY

according to ISO/IEC Guide 22 and EN 45014

Manufacturer's Name: Agilent Technologies
Manufacturer's Address: Digital Design Product Generation Unit
1900 Garden of the Gods Rd. Colorado Springs, CO 80907 USA

declares, that the product

Product Name: Trace Port Analyzer
Model Number(s): Agilent Technologies E5903A
Product Option(s): This declaration covers all options of the above product.

conforms to the following Product Specifications:

Safety: EN 61010-1:1993 / IEC 1010-1:1990+A1
UL 3111
CSA-C22.2 No. 1010.1:1993

EMC: EN 55011:1991 / CISPR 11:1990 - Group 1 Class A
IEC 555-2:1982 + A1:1985 / EN 60555-2:1987
IEC 555-3:1982 + A1:1990 / EN 60555-3:1987 + A1:1991
IEC 801-2:1991 / EN 50082-1:1992 4 kV CD, 8 kV AD
IEC 801-3:1984 / EN 50082-1:1992 3 V/m, {1kHz 80% AM, 27-1000 MHz}
IEC 801-4:1988 / EN 50082-1:1992 0.5 kV Sig. Lines, 1 kV Power Lines

Supplementary Information:

The product herewith complies with the requirements of the EMC Directive 89/336/EEC and the Low Voltage Directive 73/23/EEC and carries the CE marking accordingly.

This product was tested in a typical configuration.



Ken Wyatt / Product Regulations Manager

Colorado Springs, 8/10/98

European Contact: Your local Agilent Technologies Sales and Service Office or Agilent Technologies GmbH, Department ZQ / Standards Europe, Herrenberger Strasse 130, D-71034 Böblingen Germany (FAX: +49-7031-14-3143)

Product Regulations

Safety IEC 1010-1:1990+A1 / EN 61010-1:1993
CSA-C22.2 No. 1010.1:1993

EMC This Product meets the requirement of the European Communities (EC) EMC Directive 89/336/EEC.



ISM 1-A

Emissions EN55011/CISPR 11 (ISM, Group 1, Class A equipment)
EN60555-2 / IEC555-2
EN60555-3 / IEC555-3

Immunity EN50082-1 Code¹

IEC 801-2 (ESD) 4kV CD, 8kV AD	1
IEC 801-3 (Rad.) 3 V/m	1
IEC 801-4 (EFT) 0.5 kV, 1kV	

¹Performance Codes:

1 PASS - Normal operation, no effect.

2 PASS - Temporary degradation, self recoverable.

3 PASS - Temporary degradation, operator intervention required.

4 FAIL - Not recoverable, component damage.

Sound Pressure Level N/A

©Copyright Agilent Technologies 1994-2000

All Rights Reserved. Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under the copyright laws.

Restricted Rights Legend

Use, duplication, or disclosure by the U.S. Government is subject to restrictions set forth in subparagraph (C) (1) (ii) of the Rights in Technical Data and Computer Software Clause in DFARS 252.227-7013.

Agilent Technologies, 3000 Hanover Street, Palo Alto, CA 94304 U.S.A.

Rights for non-DOD U.S. Government Departments and Agencies are set forth in FAR 52.227-19(c)(1,2).

Document Warranty

The information contained in this document is subject to change without notice.

Agilent Technologies makes no warranty of any kind with regard to this material, including, but not limited to, the implied warranties of merchantability or fitness for a particular purpose.

Agilent Technologies shall not be liable for errors contained herein or for damages in connection with the furnishing, performance, or use of this material.

Safety

• This apparatus has been designed and tested in accordance with IEC Publication 1010, Safety Requirements for Measuring Apparatus, and has been supplied in a safe condition. This is a Safety Class I instrument (provided with terminal for protective earthing). Before applying power, verify that the correct safety precautions are taken (see the following warnings). In addition, note the external markings on the instrument that are described under "Safety Symbols."

Warning

- Before turning on the instrument, you must connect the protective earth terminal of the instrument to the protective conductor of the (mains) power cord. The mains plug shall only be inserted in a socket outlet provided with a protective earth contact. You must not negate the protective action by using an extension cord (power cable) without a protective conductor (grounding). Grounding one conductor of a two-conductor outlet is not sufficient protection.
- Only fuses with the required rated current, voltage, and specified type (normal blow, time delay, etc.) should be used. Do not use repaired fuses or short-circuited fuseholders. To do so could cause a shock or fire hazard.

- Service instructions are for trained service personnel. To avoid dangerous electric shock, do not perform any service unless qualified to do so. Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.
- If you energize this instrument by an auto transformer (for voltage reduction), make sure the common terminal is connected to the earth terminal of the power source.
- Whenever it is likely that the ground protection is impaired, you must make the instrument inoperative and secure it against any unintended operation.
- Do not operate the instrument in the presence of flammable gasses or fumes. Operation of any electrical instrument in such an environment constitutes a definite safety hazard.
- Do not install substitute parts or perform any unauthorized modification to the instrument.
- Capacitors inside the instrument may retain a charge even if the instrument is disconnected from its source of supply.
- Use caution when exposing or handling the CRT. Handling or replacing the CRT shall be done only by qualified maintenance personnel.

Safety Symbols



Instruction manual symbol: the product is marked with this symbol when it is necessary for you to refer to the instruction manual in order to protect against damage to the product.



Hazardous voltage symbol.



Earth terminal symbol: Used to indicate a circuit common connected to grounded chassis.

WARNING

The Warning sign denotes a hazard. It calls attention to a procedure, practice, or the like, which, if not correctly performed or adhered to, could result in personal injury. Do not proceed beyond a Warning sign until the indicated conditions are fully understood and met.

CAUTION

The Caution sign denotes a hazard. It calls attention to an operating procedure, practice, or the like, which, if not correctly performed or adhered to, could result in damage to or destruction of part or all of the product. Do not proceed beyond a Caution symbol until the indicated conditions are fully understood or met.

Agilent Technologies
P.O. Box 2197
1900 Garden of the Gods Road
Colorado Springs, CO 80901

Product Warranty

This Agilent Technologies product has a warranty against defects in material and workmanship for a period of one year from date of shipment. During the warranty period, Agilent Technologies will, at its option, either repair or replace products that prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by Agilent Technologies.

For products returned to Agilent Technologies for warranty service, the Buyer shall prepay shipping charges to Agilent Technologies and Agilent Technologies shall pay shipping charges to return the product to the Buyer. However, the Buyer shall pay all shipping charges, duties, and taxes for products returned to Agilent Technologies from another country.

Agilent Technologies warrants that its software and firmware designated by Agilent Technologies for use with an instrument will execute its programming instructions when properly installed on that instrument. Agilent Technologies does not warrant that the operation of the instrument software, or firmware will be uninterrupted or error free.

Limitation of Warranty

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by the Buyer, Buyer-supplied software or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

No other warranty is expressed or implied. Agilent Technologies specifically disclaims the implied warranties of merchantability or fitness for a particular purpose.

Exclusive Remedies

The remedies provided herein are the buyer's sole and exclusive remedies. Agilent Technologies shall not be liable for any direct, indirect, special, incidental, or consequential damages, whether based on contract, tort, or any other legal theory.

Assistance

Product maintenance agreements and other customer assistance agreements are available for Agilent Technologies products.

For any assistance, contact your nearest Agilent Technologies Sales Office.

Certification

Agilent Technologies certifies that this product met its published specifications at the time of shipment from the factory. Agilent Technologies further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology, to the extent allowed by the Institute's calibration facility, and to the calibration facilities of other International Standards Organization members.

About this edition

This is the *Toshiba Tx19/39 Series Emulation User's Guide*.

Publication number
E3468-97004, July 2000

Printed in USA.

New editions are complete revisions of the manual. Many product updates do not require manual changes; and, conversely, manual corrections may be done without accompanying product changes. Therefore, do not expect a one-to-one correspondence between product updates and manual updates.

UNIX is a registered trademark of The Open Group.

Windows, MS Windows, Windows NT, and MS-DOS are U.S. registered trademarks of Microsoft Corporation.

X/Open is a registered trademark, and the X device is a trademark of X/Open Company Ltd. in the UK and other countries.

Tx19/39 Embedded MIPS microprocessors are products of Toshiba, Inc.