

Printed Version of PNA Help

Agilent Technologies 4-Port N5230A Options 240 & 245 PNA Series Network Analyzers



Agilent Technologies

Manufacturing Part Number: N5230-90018

Printed in USA

Print Date: June 8, 2005

Supersedes: March 22, 2005

© Agilent Technologies, Inc. 2004 - 2005 All rights reserved.

Documentation Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED "AS IS," AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, AGILENT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. AGILENT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD AGILENT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

DFARS/Restricted Rights Notice

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as "Commercial computer software" as defined in DFAR 252.227-7014 (June 1995), or as a "commercial item" as defined in FAR 2.101(a) or as "Restricted computer software" as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies' standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Printing Copies of Documentation from the Web

To print copies of documentation from the Web, download the PDF file from the Agilent web site:

- Go to <http://www.agilent.com>.
 - Enter the document's part number (located on the title page) in the **Quick Search** box.
 - Click GO.
 - Click on the hyperlink for the document.
 - Click the printer icon located in the tool bar.
-

Contacting Agilent

This information supersedes all prior HP contact information.

Online assistance: www.agilent.com/find/assist

Americas			
Brazil <i>(tel)</i> (+55) 11 3351 7012 <i>(fax)</i> (+55) 11 3351 7024	Canada <i>(tel)</i> +1 877 894 4414 <i>(alt)</i> +1 303 662 3369 <i>(fax)</i> +1 800 746 4866	Mexico <i>(tel)</i> 1 800 254 2440 <i>(fax)</i> 1 800 254 4222	United States <i>(tel)</i> 800 829 4444 <i>(alt)</i> (+1) 303 662 3998 <i>(fax)</i> 800 829 4433
Asia Pacific and Japan			
Australia <i>(tel)</i> 1 800 802 540 <i>(fax)</i> 1 800 681 776 <i>(fax)</i> 1 800 225 539	China <i>(tel)</i> 800 810 0508 <i>(fax)</i> 800 810 0507	Hong Kong <i>(tel)</i> 800 933 229 <i>(fax)</i> 800 900 701	India <i>(tel)</i> 1600 112 626 <i>(fax)</i> 1600 113 040
Japan (Bench) <i>(tel)</i> 0120 421 345 <i>(alt)</i> (+81) 426 56 7832 <i>(fax)</i> 0120 01 2144	Japan (On-Site) <i>(tel)</i> 0120 421 345 <i>(alt)</i> (+81) 426 56 7832 <i>(fax)</i> 0120 012 114	Singapore <i>(tel)</i> 1 800 275 0880 <i>(fax)</i> (+65) 6755 1214	South Korea <i>(tel)</i> 080 778 0011 <i>(fax)</i> 080 778 0013
Taiwan <i>(tel)</i> 0800 047 669 <i>(fax)</i> 0800 047 667 <i>(fax)</i> 886 3492 0779	Thailand <i>(tel)</i> 1 800 2758 5822 <i>(fax)</i> 1 800 656 336	Malaysia <i>(tel)</i> 1800 880 399 <i>(fax)</i> 1800 801 054	
Europe			
Austria <i>(tel)</i> 0820 87 44 11* <i>(fax)</i> 0820 87 44 22	Belgium <i>(tel)</i> (+32) (0)2 404 9340 <i>(fax)</i> (+32) (0)2 404 9395	Denmark <i>(tel)</i> (+45) 7013 1515 <i>(fax)</i> (+45) 7013 1555	Finland <i>(tel)</i> (+358) 10 855 2100 <i>(fax)</i> (+358) (0) 10 855 2923
France <i>(tel)</i> 0825 010 700* <i>(fax)</i> 0825 010 701*	Germany <i>(tel)</i> 01805 24 6333* <i>(fax)</i> 01805 24 6336*	Ireland <i>(tel)</i> (+353) (0)1 890 924 204 <i>(fax)</i> (+353) (0)1 890 924 024	Israel <i>(tel)</i> (+972) 3 9288 504 <i>(alt)</i> (+972) 3 9288 544 <i>(fax)</i> (+972) 3 9288 520
Italy <i>(tel)</i> (+39) (0)2 9260 8484 <i>(fax)</i> (+39) (0)2 9544 1175	Luxemburg <i>(tel)</i> (+32) (0)2 404 9340 <i>(fax)</i> (+32) (0)2 404 9395	Netherlands <i>(tel)</i> (+31) (0)20 547 2111 <i>(fax)</i> (+31) (0)20 547 2190	Russia <i>(tel)</i> (+7) 095 797 3963 <i>(alt)</i> (+7) 095 797 3900 <i>(fax)</i> (+7) 095 797 3902
Spain <i>(tel)</i> (+34) 91 631 3300 <i>(fax)</i> (+34) 91 631 3301	Sweden <i>(tel)</i> 0200 88 22 55* <i>(alt)</i> (+46) (0)8 5064 8686 <i>(fax)</i> 020 120 2266*	Switzerland (French) <i>(tel)</i> 0800 80 5353 opt. 2* <i>(fax)</i> (+41) (0)22 567 5313	Switzerland (German) <i>(tel)</i> 0800 80 5353 opt. 1* <i>(fax)</i> (+41) (0)1 272 7373
Switzerland (Italian) <i>(tel)</i> 0800 80 5353 opt. 3* <i>(fax)</i> (+41) (0)22 567 5314	United Kingdom <i>(tel)</i> (+44) (0)7004 666666 <i>(fax)</i> (+44) (0)7004 444555		
<i>(tel)</i> = primary telephone number; <i>(alt)</i> = alternate telephone number; <i>(fax)</i> = FAX number; * = in country number 5/6/05			

This page intentionally left blank.

Whats New	30
Administrative Tasks	
PNA User Accounts and Passwords	32
Computer Properties	35
Operating System Recovery	38
Windows Considerations	41
Quick Start	
Front Panel Tour	43
Rear Panel Tour	44
Powering the PNA ON and OFF	45
PNA User Interface	48
Traces, Channels, and Windows on the PNA	50
Basic Measurement Sequence	53
Using Help	54
1. Set Up a Measurement	
Preset the PNA	62
Measurement Parameters	69
Frequency Range	75
Power Level	80
Sweep Settings	87
Trigger	96
Data Format and Scale	101
Preconfigured Measurement Setups	109
Customize Your Analyzer Screen	113
Copy Channels	121
2. Optimize a Measurement	
Dynamic Range	124
Dynamic Range-4 Jumpers	126
Dynamic Range-Test Set Option	127
Number of Data Points	128
Phase Accuracy	130
Electrically Long Devices	138
Reflection Accuracy	140
Measurement Stability	143
Noise Reduction Techniques	145
Crosstalk	151

Effects of Accessories	152
Fastest Sweep	153
Multiple State Measurements	155
Fastest Data Transfer	158
Using Macros	159
3. Calibrate a Measurement	
Calibration Overview	163
Select a Calibration	165
Calibration Wizard	168
Using Cal Sets	180
ECal	188
ECal User Characterization	195
Error Correction and Interpolation	206
Accurate Calibrations	209
Validity of a Cal	213
Measurement Errors	217
Modify Cal Kits	228
Power Calibration	243
Calibration Standards	253
TRL Calibration	257
Fixture Compensation	261
4. Analyze Data	
Locate Data Using Markers	271
Math & Memory Operations	280
Use Limits to Test Devices	284
5. Output Data	
Save and Recall Data	289
Drive Mapping	298
Print	300
Tutorials	
Network Analyzer Basics	305
Connector Care	306
ESD Protection	315
Impedance Matching Model	316
Reflected Waves	320
Reflection Measurements	321

Phase Measurements	325
Balanced Measurements	328
Amplifier Measurements	334
AM-PM Conversion	337
Antenna Measurements	341
Antenna Macro	343
Complex Impedance	347
Deviation from Linear Phase	349
Group Delay	352
Gain and Flatness	357
Gain Compression	360
Reverse Isolation	364
Absolute Output Power	366
Programming	
Command Search	
Command Finder	368
COM	
Commands	
Objects	
The Analyzer Object Model	369
Application Object	370
BalancedMeasurement Object	375
BalancedTopology Object	377
CalFactorSegments Collection	379
Calibrator Object	380
CalKit Object	384
CalManager Object	386
CalSet Object	388
CalSets Collection	392
CalStandard Object	393
Capabilities Object	395
Channel Object	397
Channels Collection	403
Fixturing Object	404
Gating Object	408
GuidedCalibration Object	410

HWAuxIO Object	412
HWExternalTestSetIO Object	414
HWMaterialHandlerIO Object	415
IIFConfiguration Object	417
IMixer Interface	419
InterfaceControl Object	422
Limit Test Collection	423
LimitSegment Object	424
Marker Object	425
Measurement Object	428
Measurements Collection	434
NAWindow Object	435
NAWindows Collection	437
Port Extension Object	438
PowerLossSegment Object	439
PowerLossSegments Collection	441
PowerSensor Object	442
PowerSensorCalFactorSegment Object	444
PowerSensors Collection	445
Preferences Object	446
SCPIStringParser Object	447
Segment Object	448
Segments Collection	450
SMC Type Object	452
SourcePowerCalibrator Object	454
Trace Object	456
Traces Collection	458
Transform Object	459
TriggerSetup Object	461
VMC Type Object	462
Properties	
AcceptTriggerBeforeArmed	464
AcquisitionDirection	465
Active Cal Kit	466
Active Channel	467
Active Marker	468

Active Measurement	469
Active NAWindow	470
ActiveXAxisRange	471
Active Trace	472
AllowArbitrarySegments	473
Alternate Sweep	474
Application	475
Arrange Windows	476
Attenuator Mode	477
Attenuator	478
AutoOrient	479
AutoPortExtConfig	480
AutoPortExtDCOffset	481
AutoPortExtLoss	482
AutoPortExtSearchStart	483
AutoPortExtSearchStop	484
AutoPortExtState	485
Averaging Count	486
Averaging Factor	487
Averaging ON/OFF	488
AvoidSpurs	489
BalancedMode	490
Bandwidth Target	491
Bandwidth Tracking	492
BB_BalPort1Negative	493
BB_BalPort1Positive	494
BB_BalPort2Negative	495
BB_BalPort2Positive	496
BBalMeasurement Property	497
Begin Response	498
Begin Stimulus	499
Bucket Number	500
C0	501
C1	502
C2	503
C3	504

Cal Factor	505
Cal Type (applied)	506
Calibration Name	508
Calibration Port	509
Calibration TypeID	510
Cal KitType	511
CalKitType (FCA)	512
Cal Power	513
Center	514
Center (Meas)	515
Center Frequency	516
Channel Number	517
CharacterizeMixerOnly	518
CharFileName	519
CharMixerReverse	520
CitiContents	521
CitiFormat	522
CmnModeZConvPortImag	523
CmnModeZConvPortReal	524
CmnModeZConvPortZ0	525
CmnModeZConvState	526
CompatibleCalKits	527
ConnectorType	528
ControlLines	529
Count	531
Couple Ports	532
CoupleChannelParams	533
Coupled Markers	534
CoupledParameters - Gate	535
CoupledParameters - Transform	536
CW Frequency	537
Delay	538
DeltaMarker	539
Description	540
DiffPortMatch_C	541
DiffPortMatch_G	542

DiffPortMatch_L	543
DiffPortMatch_R	544
DiffPortMatchMode	545
DiffPortMatchState	546
DiffPortMatchUserFilename	547
DiffZConvPortImag	548
DiffZConvPortReal	549
DiffZConvPortZ0	550
DiffZConvState	551
Display Format	552
DisplayAutomationErrors	553
DisplayGlobalPassFail	554
Distance	555
DistanceMarkerMode	556
DistanceMarkerUnit	557
Do1PortEcal	558
Do2PortEcal	559
Domain	560
DUTTopology	561
Dwell Time	562
ECALCharacterization (smc)	563
ECALCharacterization (vmc)	564
ECALCharacterizationEx	565
ECALIsolation	566
EcalOrientation	567
EcalOrientation1Port	569
EcalOrientation2Port	570
ECALPortMapEx	571
ElecDelay Medium	573
Electrical Delay	574
Embed4PortA	575
Embed4PortB	576
Embed4PortC	577
Embed4PortD	578
Embed4PortList	579
Embed4PortNetworkFilename	581

Embed4PortNetworkMode	582
Embed4PortState	583
Embed4PortTopology	584
Enabled	585
Error Correction	586
ErrorCorrection(Channel)	587
External ALC	588
ExternalTriggerConnectionBehavior	589
ExternalTriggerDelay	591
Filter BW	592
Filter CF	593
Filter Loss	594
Filter Q	595
FirmwareMajorRevision	596
FirmwareMinorRevision	597
FirmwareSeries	598
FixturingState	599
FootSwitch	600
Footswitch Mode	601
Format (Marker)	602
Format	552
Frequency	603
Frequency Span	604
FrequencyList	605
Frequency Offset Divisor	606
Frequency Offset Frequency	607
Frequency Offset Multiplier	608
Frequency Offset Override To CW	609
Frequency Offset State	610
Gate Shape	611
Gate Type	612
GPIBAddress	613
GPIB Mode	614
ID	615
IDString	616
IF Bandwidth Option	617

IF Bandwidth	618
IFDenominator	619
IFFilterSampleCount	620
IFFilterSamplePeriod	621
IFFilterSamplePeriodList	622
IFFilterSamplePeriodMode	623
IFFilterSource Property	624
IFGainLevel	625
IFGainMode	626
IFGateEnable	627
IFNumerator	628
IFSideband	629
IFSourcePath	630
IFStartFrequency	631
IFStopFrequency	632
Impulse Width	633
IndexState	634
Input A	635
Input B	636
Input C	637
InputDenominator	638
InputIsGreaterThanOrEqualToLO	639
InputNumerator	640
InputPower	641
InputStartFrequency	642
InputStopFrequency	643
InternalTestsetPortCount	644
Interpolate Correction	645
Interrupt	646
IsContinuous	647
IsECALModuleFoundEx	648
IsFrequencyOffsetPresent	649
IsHold	650
IsReceiverStepAttenuatorPresent	651
IsReferenceBypassSwitchPresent	652
IsSParameter	653

IterationsTolerance	654
Kaiser Beta	655
L0	656
L1	657
L2	658
L3	659
Label	660
LastModified	661
LimitTestFailed	662
Limit Line Begin Stimulus	499
Limit Line End Stimulus	663
Limit Line Begin Response	498
Limit Line End Response	664
Limit Type	665
Line Display	666
LoadCharFromFile	667
LoadPort	668
LocalLockoutState	669
LODenominator	670
LOFixedFrequency	671
LOName	672
LONumerator	673
LOPower	674
LORangeMode	675
Loss	676
Loss (sourceCal)	677
LOStage	678
LOStartFrequency	679
LOStopFrequency	680
MagnitudeOffset	681
MagnitudeSlopeOffset	682
Marker Bucket Number	500
Marker Format (all)	683
Marker Format (indiv)	602
Marker Interpolate(all)	684
Marker Interpolate (indiv)	685

Marker Number	686
MarkerReadout	687
MarkerReadoutSize	688
MarkerState	689
Marker Type	690
Marker X-axis Value	691
Marker Y-axis Value	692
Maximum Frequency	693
MaximumFrequency (capabilities)	694
MaximumFrequency (sourceCal)	695
MaximumIFFilterSampleCount	696
MaximumIterationsPerPoint	697
MaximumNumberOfPoints	698
MaximumReceiverStepAttenuator	699
MaximumSourceALCPower	700
MaximumSourceStepAttenuator	701
Mean	702
Medium	703
Minimum Frequency	704
MinimumFrequency (capabilities)	705
MinimumFrequency (sourceCal)	706
MinimumIFFilterSampleCount	707
MinimumNumberOfPoints	708
MinimumReceiverStepAttenuator	709
MinimumSourceALCPower	710
Name (meas)	711
Name (trace)	712
Name (CalKit object)	713
Number (meas)	714
Number of Points	715
Number of Points (Meas)	716
NumberOfPorts	717
NumberOfPorts(Testset)	718
OmitIsolation	719
OneReadoutPerTrace	720
Options	721

OrientECALModule	722
OutputFixedFrequency	723
OutputPort	724
OutputSideband	726
OutputStartFrequency	727
OutputStopFrequency	728
Parameter	729
Parent	730
PassFailLogic	732
PassFailMode	733
PassFailPolicy	734
PassFailScope	735
PassFailStatus	736
Peak Excursion	737
Peak Threshold	738
PeakTo Peak	739
Phase Offset	740
Port 1	741
Port 2	742
Port 3	743
Port2PdeembedCktModel	744
Port2PdeembedState	745
PortArbzImag	746
PortArbzReal	747
PortArbzState	748
PortArbzZ0	749
PortCLogic	750
PortCMode	751
PortDelay	752
PortExtState	753
PortExtUse1	754
PortExtUse2	755
PortFreq1	756
PortFreq2	757
Port Label	758
PortLogic	759

PortLoss1	760
PortLoss2	761
PortLossDC	762
PortMatching_C	763
PortMatching_G	764
PortMatching_L	765
PortMatching_R	766
PortMatchingCktModel	767
PortMatchingState	768
PortMode	769
Power Slope	770
Power Acquisition Device	771
Power Meter Channel	772
Power Meter GPIBAddress	773
R1 Input Path	774
Readings Per Point	775
ReadingsTolerance	776
ReadyForTriggerState	777
Receiver Attenuator	778
ReceiverCount	779
ReceiverStepAttenuatorStepSize	780
Receive Port	781
ReduceIFBW	782
ReferenceCalFactor	783
Reference Marker State	784
Reference Level	785
Reference Position	786
SB_BalPortNegative	787
SB_BalPortPositive	788
SB_SEPort	789
SBalMeasurement	790
Scope	791
Search Function	792
SecurityLevel	793
Segment Number	794
Show Statistics	795

ShowProperties	796
SICL	797
SICLAddress	798
Simultaneous2PortAcquisition	799
Smoothing Aperture	800
Smoothing ON/OFF	801
SnPFormat	802
Sound On Fail	803
SourceCount	804
Source Port	805
Source	806
SourcePowerCalPowerOffset	807
Source Power Correction	808
Source Power Option	809
Source Power State	810
Span	811
Span (Meas)	812
SSB_BalPortNegative	813
SSB_BalPortPositive	814
SSB_SEPort1	815
SSB_SEPort2	816
SSBMeasurement	817
Standard Deviation	818
Standard For Class	819
Start Frequency	821
Start Power	822
Start	823
Start (Meas)	824
State	825
Statistics Range	826
Step Rise Time	827
StimulusValues	828
Stop Frequency	829
Stop Power	830
Stop	831
Stop (Meas)	832

strPort2Pdeembed_S2PFile	833
strPortMatch_S2PFile	834
SweepEndMode	835
SweepHoldOff	836
Sweep Generation Mode	837
Sweep Time	838
Sweep Type	839
System Impedance Z0	840
SystemName	841
Target Value	842
Test Port Power	843
ThruCalMethod (FCA)	844
ThruCalMethod	845
ThruPortList	846
Title	847
Title State	848
Trace Math	849
Tracking	850
Transform Mode	851
Trigger Delay	852
TriggerOutputEnabled	853
Trigger Mode	854
Trigger Signal	855
Trigger Type	856
Type (calstd)	857
TZImag Property	858
TZReal Property	859
UnusedChannelNumbers	860
UsedChannelNumbers	861
Use Power Loss Segments	862
Use Power Sensor Frequency Limits	863
User Range	864
User Range Max	865
User Range Min	866
UserPresetEnable	867
ValidConnectorType	868

Velocity Factor	869
View	870
Visible	871
WGCutoffFreq	872
Window Number	873
Window State	874
XAxis Point Spacing	875
YScale	876
Z0	877
Methods	
Abort	878
AbortPowerAcquisition	879
Acquire Cal Standard	880
Acquire Cal Standard2	882
AcquireCalConfidenceCheckECALEX	884
AcquirePowerReadings	885
AcquireStep	886
Activate	887
Activate Marker	888
Activate Window	889
Add (channels)	890
Add (measurement)	891
Add (naWindows)	892
Add (PowerLossSegment)	893
Add (PowerSensorCalFactorSegment)	894
Add (segments)	895
Allow All Events	896
Allow Event Category	897
Allow Event Message	898
Allow Event Severity	899
Apply	900
ApplyPowerCorrectionValues	901
AutoPortExtMeasure	902
AutoPortExtReset	903
Autoscale	904
Averaging Restart	905

Build Hybrid Kit	906
Calculate Error Coefficients	907
Calculate	908
Change Parameter	910
CheckPower	912
Close CalSet	913
ComputeErrorTerms	914
ConfigNarrowBand2	915
ConfigurationFile	917
Continuous Sweep	918
Copy	919
CopyToChannel	920
Create SParameterEX	921
CreateCalSet	922
CreateCustomMeasurementEx	923
Create Custom Cal	925
Create Measurement	926
DataToMemory	928
Delete	929
Delete Marker	930
Delete All Markers	931
DeleteCalSet	932
Delete ShortCut	933
Delta Marker	539
Disallow All Events	934
Do Print	935
DoECAL1PortEx	936
DoECAL2PortEx	937
DoneCalConfidenceCheckECAL	938
DoReceiverPowerCal	939
Execute	940
Execute Shortcut	941
GenerateErrorTerms	942
GenerateSteps	943
Get AuxIO	944
Get Cal Standard	945

Get CalManager	946
Get CalSetByGUID	947
Get CalSetCatalog	948
Get CalSetUsageInfo	949
Get Cal Types	950
Get Complex	951
Get DataByString	952
Get Data	954
Get ECALModuleInfoEx	956
Get Error Term	957
Get ErrorTerm2	959
Get Error Term By String	961
Get Error Term Complex	962
Get Error Term Complex2	964
Get Error Term Complex By String	966
Get Error Term List	968
Get Error Term List2	970
Get ExternalTestSetIO	971
Get Filter Statistics	972
Get Guid	973
Get Input Voltage	974
Get Input1	975
Get MaterialHandlerIO	976
Get NAComplex	977
GetNumberOfGroups	978
Get Output	979
Get Output Voltage	980
Get OutputVoltage Mode	981
Get Paired Data	982
Get Port	984
Get PortC Data	985
Get Reference Marker	986
Get Required Eterm Names	987
Get Scalar	988
Get Shortcut	990
Get SnPData	991

Get SourcePowerCalDataEx	993
Get SourcePowerCalDataScalarEx	994
Get Standard	996
Get Standard By String	998
Get Standard Complex	999
Get Standard Complex By String	1001
Get StandardsList	1002
Get Standard List2	1004
Get StandardsForClass	1005
Get StepDescription	1007
Get Test Result	1008
Get Trace Statistics	1009
Get X-Axis Values	1010
GetXAxisValues (Meas)	1011
Get X-axis Values Variant	1012
Has CalType	1013
Hold	1015
Hold (All Chans)	1016
Initialize	1017
Item	1018
LaunchCalWizard	1020
LaunchPowerMeterSettingsDialog	1021
LoadFile	1022
Manual Trigger	1023
MessageText	1024
Next IF Bandwidth	1025
Number of Groups	1026
Open CalSet	1027
Parse	1029
Preset (app and chan)	1030
Previous IF Bandwidth	1031
Print To File	1032
Put Complex	1033
Put Data Complex	1035
Put ErrorTerm	1037
Put ErrorTerm2	1039

Put Error Term By String	1040
Put ErrorTerm Complex	1041
Put ErrorTerm Complex2	1043
Put Error Term Complex By String	1044
Put Formatted Scalar Data	1045
Put NAComplex	1046
Put Output	1048
Put Output Voltage	1049
Put Output Voltage Mode	1050
Put Port	1051
Put PortCData	1053
Put Scalar	1054
Put Shortcut	1056
Put SourcePowerCalDataEx	1057
Put SourcePowerCalDataScalarEx	1058
Put Standard	1059
Put Standard By String	1061
Put Standard Complex	1062
Put Standard Complex By String	1064
Quit	1065
Read Data	1066
Read Raw	1067
Recall	1069
Recall Kits	1070
Remove	1071
Reset	1072
Restore Cal Kit Defaults	1073
Restore Cal Kit Defaults All	1074
Resume	1075
Save	1076
Save (CalSet)	1077
Save CalSets	1078
SaveCitiDataData	1079
SaveCitiFormattedData	1080
Save File	1081
Save Kits	1082

Search Filter Bandwidth	1083
Search Max	1084
Search Min	1085
Search Next Peak	1086
Search Peak Left	1087
Search Peak Right	1088
Search Target	1089
Search Target Left	1090
Search Target Right	1091
SelectCalSet	1092
Set All Segments	1093
Set BBPorts	1094
Set Cal Info	1095
SetCallInfo2 (power)	1097
Set Center	1099
Set CW	1100
Set Electrical Delay	1101
Set FailOnOverRange	1102
SetPowerAcquisitionDevice	1103
Set Frequency LowPass	1104
Set Reference Level	1105
Set SBPorts	1106
Set SSBPorts	1107
Set StandardsForClass	1108
Set Start	1110
Set Stop	1111
Show Marker Readout	1112
Show Status Bar	1113
Show Stimulus	1114
Show Table	1115
Show Title Bars	1116
Show Toolbar	1117
Single	1118
StringToNACalClass	1119
StringtoNAErrorTerm2	1121
UserPreset	1122

UserPresetLoadFile	1123
UserPresetSaveState	1124
Write Data	1125
Write Raw	1126
Events	
OnCalEvent	1128
OnChannelEvent	1129
OnDisplayEvent	1130
OnHardwareEvent	1131
OnMeasurementEvent	1132
OnSCPIEvent	1133
OnSystemEvent	1134
OnUserEvent	1135
Examples	
CalSet_Examples	1136
Getting Trace Data from the Analyzer	1138
Perform a Source Power Cal	1141
Upload a Source Power Cal	1144
Upload Segment Table	1146
Create and Cal an SMC Measurement	1148
Create and Cal a VMC Measurement	1150
Create an SMC Fixed Output Meas	1153
Create a Pulsed Measurement	1155
Perform an ECAL Confidence Check	1157
Limit Line Testing Example with COM	1159
Events Example	1160
Concepts	
Configure for COM-DCOM Programming	1161
COM Fundamentals	1166
Getting a Handle to an Object	1169
Collections in the Analyzer	1172
COM Data Types	1173
PNA Automation Interfaces	1175
Working with the Analyzer's Events	1176
Read and Write Calibration Data using COM	1180
C and the COM Interface	1181

Using .NET	1184
SCPI	
Commands	
List of SCPI Commands	1186
SCPI Command Tree	1201
Common Commands	1203
Abort	1206
Calculate	
Correction	1207
Custom	1213
Data	1216
Filter	1221
Format	1226
FSimulator	1227
Function	1228
Limit	1233
Marker	1238
Math	1254
Mixer	1256
Normalize	1257
Offset	1260
Parameter	1262
RData	1267
Smoothing	1268
Transform	1270
Control	1279
Display	1285
Format	1300
Hardcopy	1302
Initiate	1303
Memory	1305
Output	1314
Route	1315
Sense	
Average	1316
Bandwidth	1318

Correction	
Correction	1320
Guided Cal	1334
Cal Kit	1343
Cal Stds	1346
Cal Sets	1367
Extensions	1375
Session	1384
SMC	1389
VMC	1395
Couple	1404
Frequency	1406
IF	1410
Mixer	1415
Offset	1432
Power	1436
Roscillator	1437
Segment	1438
Sweep	1448
XAxis	1455
Source	1456
Source Correction	1463
Status	1477
System	1491
Trigger	1501
Examples	
Catalog Measurements	1504
Create a measurement	1505
Channels, Windows, and Measurements using GPIB	1506
Setup Sweep Parameters	1508
Setup the Display	1509
Perform a Guided Cal	1511
Perform Guided ECal	1514
Perform Guided Mechanical Cal	1516
Perform Guided 1Port	1517
Perform Unguided ECAL	1519

Perform Unguided 2-Port Mech Cal	1520
Perform an Unguided 1-Port Cal on Port 2	1522
Perform an ECAL Confidence Check	1524
Perform a Source Power Cal	1527
Uploading a Source Power Cal	1533
Perform a Sliding Load Cal	1537
Create New Cal Kit using SCPI	1538
Modify a Calibration Kit	1544
Create and Cal a VMC Measurement	1150
Create and Cal an SMC Measurement	1148
Create an SMC Fixed Output Measurement	1551
Getting and Putting Data using GPIB	1554
Getting and Putting Data (definite block transfers)	1556
Transfer Data using GPIB	1559
Establish a VISA Session	1561
Status Reporting	1563
GPIB using Visual C	1565
Create a Custom Power Meter Driver	1569
GPIB Pass Through	1572
PNA as Controller and Talker/Listener	1573
Concepts	
GP-IB Fundamentals	1575
The Rules and Syntax of SCPI Commands	1581
Getting Data from the Analyzer	1585
Understanding Command Synchronization	1588
Reading the Analyzer's Status Registers	1593
Configure for VISA and SICL	1596
Data Access Map	
Data Map	1599
Rear Panel IO Connectors	
Interface Control	1600
Auxiliary IO connector	1606
External TestSet IO Connector	1611
Material Handler IO Connector	1616
COM versus SCPI	1629
Using Macros	159

Time Domain	
Time Domain	1631
Frequency Offset (Opt 080)	
Frequency Offset (Option 080)	1645
Frequency Converting Device Measurements	1652
Frequency Offset Calibration	1653
Conversion Loss	1655
Conversion Compression	1658
Isolation	1660
Harmonic Distortion	1663
Return Loss and VSWR	1665
Frequency Converter Application (Opt 083)	
Known Issues	1667
Overview	1668
Using the Frequency Converter Application	1669
Calibrations	1677
Configure a Mixer	1691
Configure an External LO Source	1699
High Power Measurements	
External Leveling Circuit	1704
High-Power Measurements	1705
E835x Standard	
Diagram: Basic Config	1715
Diagram 1: Fwd Msmts	1716
Diagram 2: Fwd Msmts	1717
Diagram 1: Fwd & Rev Msmts	1718
Diagram 3: Fwd & Rev Msmts	1719
Diagram 1: Booster amp	1720
Diagram 2: Booster amp	1721
Diagram 3: 2 Booster amps	1722
Diagram 1: Ext level	1723
Diagram 2: Ext level	1724
Diagram 3: Ext level	1725
Diagram: Cal Power Levels	1726
E835x Opt 015	
Diagram: Basic Config	1727
Diagram 1: Fwd Msmts	1728

Diagram 2: Fwd Msmts	1729
Diagram: Fwd & Rev Msmts	1730
Diagram 1: Booster amp	1731
Diagram 2: Booster amp	1732
Diagram 1: Ext level	1733
Diagram 2: Ext level	1734
Diagram: Cal Power levels	1735
E836x Standard	
Diagram: Basic Config	1736
Diagram: Fwd Msmts	1737
Diagram: Fwd & Rev Msmts	1738
Diagram: Booster amp	1739
E836x Opt 014	
Diagram: Basic Config	1740
Diagram 1: Fwd Msmts	1741
Diagram 2: Fwd Msmts	1742
Diagram 1: Booster amp	1744
Diagram 2: Booster amp	1746
Diagram: Fwd & Rev Msmts	1748
Diagram: Cal Power Levels	1750
E880x Standard	
Diagram: Basic config	1751
Diagram: Fwd Msmts	1752
Diagram: Fwd & Rev Msmts	1753
Diagram: Booster amp	1754
Diagram: Ext Level	1755
E880x Opt 014	
Diagram: Basic Config	1756
Diagram 1: Fwd Msmts	1757
Diagram 2: Fwd Msmts	1758
Diagram: Fwd & Rev Msmts	1759
Diagram 1: Booster amp	1760
Diagram 2: Booster amp	1761
Diagram 1: Ext level	1762
Diagram 2: Ext level	1763
Diagram: Cal Power Levels	1764
N338x Standard	

Diagram: Basic Config	1765
Diagram: Fwd Msmts	1766
Diagram: Fwd & Rev Msmts	1767
Diagram: Booster amp	1768
Diagram: Ext level	1769
N338x Opt 014	
Diagram: Basic Config	1770
Diagram 1: Fwd Msmts	1771
Diagram 2: Fwd Msmts	1772
Diagram: Fwd & Rev msmts	1773
Diagram 1: Booster amp	1774
Diagram 2: Booster amp	1775
Diagram 1: Ext level	1776
Diagram 2: Ext level	1777
Diagram: Cal Power Levels	1778
Networking the PNA	
Drive Mapping	298
Easy vs Secure Configuration	1779
Changing Network Client	1780
Product Support	
Troubleshoot the PNA	1781
List of Error Messages	1784
About Error Messages	1840
Accessories	1843
USB to GPIB Adapter	1850
Firmware Update	1853
PNA Configurations and Options	1858
Option Enable	1864
Other Resources	1867
SCPI Errors	1869
Technical Support	1879
Diagnostic Tools and Adjustments	
3.8 GHz Frequency Adjust	1884
10 MHz Reference Adjust	1886
LO Power Adjust	1888
Offset LO Power Adjustment	1890

Operators Check	1891
Option H11 Verification	1893
Phase-Lock IF Gain Adjust	1896
System Verification	1897
Source Cal	1907
Receiver Cal	1910
Receiver Display	1913
Serial Bus Test	1914
Instrument Calibration	1915
IF Access Applications (Opt H11)	
About the H11 Option	1916
External Test Head Configuration	1918
Pulsed Application	1922
Controlling External Devices	
Analyzer Accessories	1843
E5091 Test Set Control	1932
Interface Control	1600
USB to GPIB Adapter	1850
Aux IO Connector	1606
Handler IO Connector	1616
Test Set IO Connector	1611
Configure an External LO Source	1699
Specifications	
E8356A, 57A, 58A	1935
E8801A, 02A, 03A	1965
N3381A, 82A, 83A	1989
E8361A	2014
E8362A, 63A, 64A	2068
E8362B, 63B, 64B	2069
N5230A 2-Port	2111
N5230 4-Port	2178
N5250A	2205
Glossary	2211

What's New in PNA Code Version 5.25

- [TRL Calibration](#)
- [Dedicated calibration window](#)
- [Calibration Class Label](#)
- [Data-Based Cal Kits can now be modified](#)
- [Guided SmartCal supports ECal on one or more ports.](#)
- [Option H11 Verification](#)
- [Safely shutdown the PNA without a mouse](#)

See [New 5.25 Programming Commands](#)

To check your PNA code version, click **Help**, then **About Network Analyzer**

What's New in PNA Code Version 5.22

- [New *.csa Save/Recall File Type](#)
- [4-Port Fixture Simulator Functions](#)
 - [4-Port Network Embed/De-embed](#)
 - [Balanced Conversion](#)
 - [Differential / Common Mode Port Z Conversion](#)
 - [Differential Matching Circuit Embedding](#)
- [Automatic Port Extensions](#)
- [Interface Control](#)
- [Agilent 5091A Testset Control](#)
- [8 Traces per Window \(previously 4\)](#)
- [CA on Status Bar](#)
- [.PDF version of this Help file available](#)

See [New 5.22 Programming Commands](#)

What's New in PNA Code Version 5.0

- New 4-port PNA Models:

- N5230A Options 240 and 245
- Balanced Measurements
- Calibration Registers
- Number of User Ranges (Stats and Markers) expanded to 16
- Port Extension Toolbar and Additional Features
- Magnitude Offset
- 2-Port Fixture Compensation
- Pulse Profile - S-Parameters
- Two LO Sources for Millimeter Wave Measurements
- Material Handler Trigger Control. Also available using SCPI, and COM
- Global Pass / Fail Dialog Also available using SCPI and COM.
- Revised Operator's Check
- Revised System Verification
- Guided Calibration COM Interface

See New 5.0 Programming Commands

PNA User Accounts and Passwords

When the PNA power is switched on, it automatically logs into Windows using the default user name and password. This gives anyone full access to the analyzer. The following steps can be taken to increase security of your PNA.

- Require users to logon when the PNA computer is turned ON - [Learn how to enable this feature](#)
- Setup individual accounts on the PNA with varying level of access - Learn how to [Add or Change User Accounts and Passwords](#)

[Please read about Anti-virus protection for your PNA](#)

Existing User Accounts

The following user accounts already exist on new PNAs:

- **Default User Account**
Beginning in April 2004, PNAs were shipped from the factory with the default user name is **PNA-Admin** and the password is **agilent**.
For PNAs shipped before that, the default user name is **Administrator** and the password is either **tsunami** or left blank.
These accounts are created by Windows and cannot be deleted.
We recommend you change the password and, if desired, the user name.
DO NOT FORGET YOUR NEW PASSWORD. You will not be able to start your PNA without it.
- **Agilent Account** This Administrator account is created by Agilent for service purposes. Each PNA has a unique password for this account. Although allowed by Windows, please do not delete this account.
- **Guest Account** This account allows anyone to type in any name, without password, and gain limited access to the PNA files. This account is created by Windows and cannot be deleted. It can be renamed. This account is turned OFF when the PNA is shipped.

Notes



- Although allowed by Windows, do NOT setup an Administrator account without a password. Internet viruses look for, and exploit, this condition.
- You can create as many user accounts as you like.
- The user name is not case sensitive. The password IS case sensitive.
- The PNA local policies are set so that, if logon is required, you must retype the user name (and password) every time. Do not change the local policies on the PNA.

How to Require Users to Logon when the PNA Computer is turned ON.

[How do I know which Operating System I have?](#)

Windows 2000	Windows XP
On the Windows taskbar, click Start , then Settings , then Control Panel	On the Windows taskbar, click Start , then Run
Double click Users and Passwords	Type control userpasswords2 then click OK
Check Users must enter a user name and password to use this computer.	Check Users must enter a user name and password to use this computer.

To turn this function OFF, perform the same procedure, but clear the checkbox. The account that is selected when the checkbox is cleared is the account that is automatically logged on when the PNA is turned ON.

Add or Change User Accounts and Passwords

If the analyzer is in a secure environment, you can setup PNA users by name and grant various levels of access. This is particularly important when the PNA is remotely controlled or accessed over LAN.

You can designate a person as the administrator and then configure the PNA to allow others to use it with reduced permissions. That is, other people can be signed on to use the analyzer but they will not have the ability to perform all of the administrative functions that you can as the administrator.

How to add or change a user account and password

How do I know which Operating System I have?

Windows 2000	Windows XP
In the analyzer System menu, point to Configure , and click Control Panel .	Click Start, then point to Settings, then click Control Panel
In the Control Panel window, scroll down and select the Users and Passwords application.	Click User Accounts
On the Users tab, if the Add button appears dimmed, select the Users must enter a user name and password to use this computer check box near the top of the window.	Follow the prompts to: <ul style="list-style-type: none"> • Change an account • Create a new account • Change the way users log on or off.
Click Add to enter the information for yourself or for another user.	CAUTION: Although allowed by Windows, do NOT allow an Administrator account without a password. Internet viruses look for, and exploit, this condition.
In the User name box, enter a user name for the user. In the Full name box, enter the full name of the user.	
In the Description box, enter a description for the user. Then, click Next .	

<p>In the Password box, have the user type a password. Have the user retype the password in the Confirm password box. Then, click Next.</p>	
<p>Select the level of access that you wish to grant this user.</p> <p>Note: Standard users and restricted users are unable to switch GPIB modes and install firmware.</p> <p>There are several other levels of security that you may grant in the Other list. A description of each of these other levels is displayed beneath the Other box when it is selected. Then, click Finish.</p>	
<p>In the Users for this computer box, validate the user name and security level group of the user.</p>	
<p>If you want this user to be able to use the network analyzer without entering their password each use, clear the Users must enter a user name and password to use this computer check box. Click OK.</p>	
<p>When the Automatically Log On window is displayed, have the new user type their password in the Password box and have them retype the password in the Confirm Password box.</p>	
<p>Click OK to complete this user addition.</p>	
<p>In the File menu, click Close to close the Control Panel.</p>	

PNA Computer Properties

The PNA uses a personal computer and a Windows operating system. The following are common tasks that you may need to perform on the PNA computer.

[View or change Full Computer Name](#)

[Check IP Address](#)

[Check the amount of RAM](#)

[Check CPU Speed](#)

[Set Time and Date](#)

Other Administrative Task Topics

View or change Full Computer Name

Your PNA has a unique computer name that identifies it on a network. To view or change the computer name, you must first minimize the PNA application.

How do I know which Operating System I have?

Windows 2000	Windows XP
On the desktop, right-click My Computer	On the desktop, right-click My computer Icon
Click Properties	Click Properties
Click the Network Identification tab at the top of the dialog box	Click the Computer Name tab at the top of the dialog box
Click Properties	Click Change next to "..rename this computer.." message
Type your new Computer Name	Type your new Computer Name

Note: To add your computer to a domain, or to set up the networking configuration, contact your company's I.T. department. This setup is custom for each company.

To restore the PNA application, click **PNA Analyzer** in the task bar at the bottom of the screen.

Check IP Address

If your PNA is connected to a LAN, you can view the IP address and other networking information.

1. Minimize the PNA application
2. Click **Start**, then **Run**
3. Type **cmd**, then click **OK**

- At a DOS prompt, type **ipconfig /all**

Check the amount of RAM

Random Access Memory (RAM) is the amount of working memory in your computer. The PNA application can require up to 512 MB of RAM depending on the settings you use. If your PNA is operating slowly when you have more than four windows open or if you routinely use more than 1601 data points, you may need to upgrade to 512 MB.

To view the amount of PNA RAM, you must first minimize the PNA application.

How do I know which Operating System I have?

Windows 2000	Windows XP
On the desktop, right-click My Computer	On the desktop, right-click My computer Icon
Click Properties	Click Properties
Click the General tab at the top of the dialog box	Click the General tab at the top of the dialog box
The amount of RAM appears at the bottom of the window.	The amount of RAM appears at the bottom of the window.

To restore the PNA application, click **PNA Analyzer** in the task bar at the bottom of the screen.

Check CPU Speed

The speed of the PNA processor (CPU) is a factor in determining how quickly the PNA processes data. See PNA configurations to learn if you can upgrade your PNA CPU. To check your PNA CPU speed, you must first minimize the PNA application.

How do I know which Operating System I have?

Windows 2000	Windows XP
On the desktop, right-click My Computer	On the desktop, right-click My computer Icon
Click Manage	Click Properties
Open System Tools folder, then click System Information .	Click the General tab at the top of the dialog box
Click System Summary .	The CPU speed appears near the bottom of the window
After refreshing, the CPU speed appears at the end of the Processor entry.	

To restore the PNA application, click **PNA Analyzer** in the task bar at the bottom of the screen.

Set Time and Date

Both Windows 2000 and XP

To set the time and date on your PNA, you must first minimize the PNA application.

1. Move the cursor to the lower corner of the screen
2. When the taskbar appears, double-click on the displayed time. This opens the **Date/Time Properties** dialog box.
3. Change the date, time, and time zone as appropriate.

To restore the PNA application, click **PNA Analyzer** in the task bar at the bottom of the screen.

Recovering from PNA Hard Drive Problems

The leading cause of PNA failures is problems with the PNA Hard Disk Drive (HDD). These problems are usually preventable (see [Preventing PNA HDD Problems](#)), and in many cases, recoverable. The following could save you weeks of downtime and the cost of replacing your PNA HDD.

The following three symptoms indicate a probable HDD failure. First, attempt to perform an [Operating System Recovery](#). If it fails, the HDD must be replaced.

1. Will not complete the boot process.
 - If 'Couldn't find NTLDR' appears, remove if a disk is in the PNA floppy drive.
 - If 'Operating System not found' appears, replace the HDD.
2. Continual blue screens or multiple errors.
3. Excessive clicking or a loud high-pitch whine.
 - Back up files and replace HDD.

The following three symptoms indicate missing or corrupt files. First, try the suggestions indicated by bullets. Then, perform an [Operating System Recovery](#)., which is likely to solve the problem.

1. Required system files are not found.
2. The operating system or PNA application does not function properly.
 - Uninstall the PNA application using Add/Remove Programs from the Control Panel. Then reinstall the PNA application by double-clicking on D:\Updates\Firmware*.msi. or download a firmware update using AgileUpdate.
3. The PNA functions, but is very slow.
 - Check for excessive clicking or a loud high-pitch whine (see #3 above).
 - Check RAM. For best performance, RAM must be at least 128MB for PNA firmware rev. 3.0 or below; 256MB for firmware rev. 3.1 or higher. See PNAHelp to learn more.
 - Scan for Virus and "spyware".

Operating System Recovery

This procedure will completely restore the operating system of the PNA back to the original factory condition. It will not work if the hard drive is damaged.

Important note: This procedure will overwrite the entire C: drive and the following information will be lost:

- All changes and additions made to the analyzer since purchase (except options)
- All user accounts and passwords
- All added programs
- All saved instrument states

- All user configurations and Windows settings

You can save this information to a floppy drive or to a folder on the D:drive. The D:drive will not be affected by this restoration process. In addition, factory instrument calibration will not be affected if no changes have been made since the original factory calibration. If changes have been made through the service routines, copy all files that start with "mxcalfile_" in the C:\Program Files\Agilent\Network Analyzer directory, and save them to the D:\Calfiles directory.

Procedure

1. Click **Start, Shutdown, Restart**
2. After the Agilent logo, when '**Please select the operating system to start:**' displays, quickly press the down arrow on the keyboard to select the System Recovery partition, (NOT the Recovery Console). Press **Enter**.
NOTE: If you do not reach this screen during the boot process, you may be able to boot from a floppy disk. See [If you CANNOT boot from the Hard Drive](#) below.
3. The PNA will display a warning about proceeding and give you two chances to abort. After the second warning, the restoration process will begin immediately.
4. Restoration takes from 15 to 45 minutes. There is no user interaction required. Near the end of the process, the PNA may reboot several times. Do not attempt to use the analyzer until the PNA application is running and all activity has stopped for at least one minute.
5. Once the operating system is completely recovered, you can restore any files you may have saved back to their original locations. The mxcalfiles that were stored in D:\Calfiles will be restored automatically. Other files must be copied or moved manually.
6. If PNA application updates had previously been downloaded through AgileUpdate, they can now be re-installed. Double-click on D:\Updates\Firmware*.msi. or download a firmware update using AgileUpdate.

If you CANNOT boot from the Hard Drive

During the boot process, you may not reach the screen that displays '**Please select the operating system to start**'. You may be able to boot from a floppy disk if your PNA Hard drive is labeled 'S.02.xx' and 'S.05.50'. If labeled with a different code, the process will fail at step 2 below, but no further damage will be done.

Make this disk using a computer that is currently running DOS or Windows 95/98/ME/XP. Note: Windows NT or 2000 cannot be used.

To create this disk, right-click on the A: drive in Windows Explorer, select **Format**, then select **Make System Disk**. This may be called **copy system files**, or **Create an MS-DOS startup disk**.

To boot from this disk:

1. Insert the created system disk into the PNA and restart. The PNA should detect the floppy disk and boot from it. See below if it does NOT boot.
2. At the DOS prompt (A:\>)type CD C: and press Enter. You are really changing to the D: drive because a DOS operating system does not recognize the NTFS format and assumes the first valid drive is C:.
3. Type **C:\minint\bin\recovery.bat** and press **Enter**. If this returns an error, type **C:\Autoexec.bat**
4. Continue with Operating System Restoration [Procedure](#) (above).

If the PNA does not Boot from the floppy, then change the PNA Bios settings. Due to bios revisions, this procedure may vary slightly from the following:

1. Restart the PNA.
2. When the Agilent logo appears, press F2 (function key) on the keyboard a few times. The Bios menu will appear after several seconds.
3. Select **Boot** using the keyboard arrows. Read "Item Specific Help" to learn to move the **Removable Devices / floppy drive** to a boot position before the **Hard Drive**.
4. Select **Save** then **Exit**.
5. To prevent an error message when a floppy disk is inserted while powering up, use this procedure to change back to booting from the hard drive.

Microsoft Windows[®] XP / 2000 Considerations

Critical Notes

Windows Operating System

Note: Beginning in April 2004, the PNA is shipped from the factory with a modified version of Microsoft Windows XP operating system. Previously, the PNA was shipped with Windows 2000. The PNA application performs identically using these two operating systems.

To determine which Operating System is installed on your PNA:

1. Minimize the PNA application
2. On the PNA desktop, click Start.
3. Along the side of the Start menu appears one of the following:
 - **Windows 2000 Professional**
 - **Windows XP Professional**


VERY IMPORTANT information to protect your hard drive!

The leading cause of PNA failures is problems with the PNA Hard Disk Drive (HDD). These problems are usually preventable, and in many cases, recoverable. [Learn more about protecting your PNA.](#)

Using USB

The PNA has at least two USB ports for connecting devices: one on the front panel and at least one on the rear panel. The main advantages of USB are “hot” connects and disconnects and fast data transfer speeds. Electronic Calibration modules are now available with USB connections.

The first time you plug a device into a USB port there is some wait time. Windows reports it is identifying the hardware, then searching for the correct driver, then installing the driver (if it was found).

 Connecting that same device back into that same port later is quick and easy, but if you move the device to a different USB port, you will have to wait through the hardware ID and driver search again.

Note: Certain USB devices (such as ECAL modules) require you be logged on with Administrator privileges the first time you plug them into the PNA. This must be done for each serial number. Click **Next** to choose the default settings when installing new USB devices.

Plug & Play Stability and Security

Plug & Play capabilities is similar to Win 95 and 98. It provides both a stable and secure operating environment. You may notice also that it greatly reduces the number of required reboots.

LAN Connections

Windows supports DHCP and fixed IP addressing. Also, “Hot” connect and disconnect of the LAN cable, as well as a visual indicator of LAN status in system tray area, makes LAN connections more intuitive. In addition, the Hardware Wizard helps users with system hardware configuration.

Single and Double Click option.


By default, Windows allows a single-click method of launching icons. To revert to double-clicking, click **Start**, then **Settings**, then **Control Panel**, then click **Mouse**. In the Mouse Properties dialog, select **Double-click to open an item**. Then click **OK**.

Printing

Adding a printer should be done outside of the PNA application. [Learn more.](#)


Front Panel Tour

Click on the sections of the front panel for information.

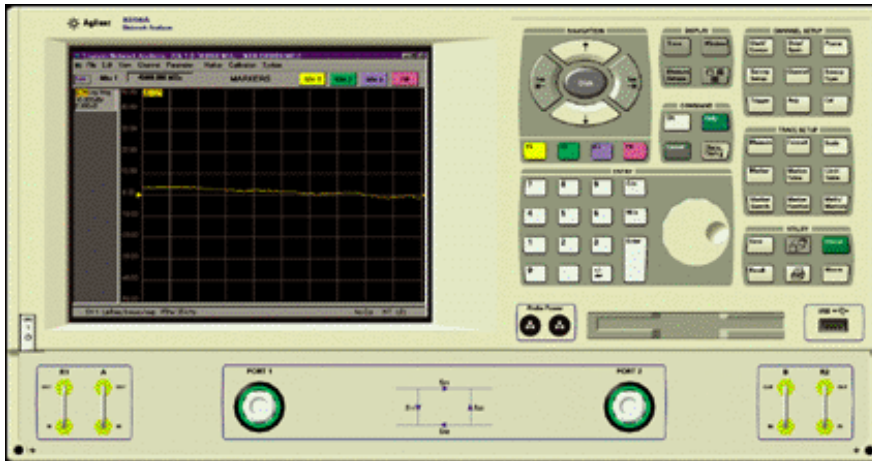

Rear Panel Tour

This image includes ALL rear-panel features.
Your PNA may not have this capability or look.
Click on a connector for detailed information.

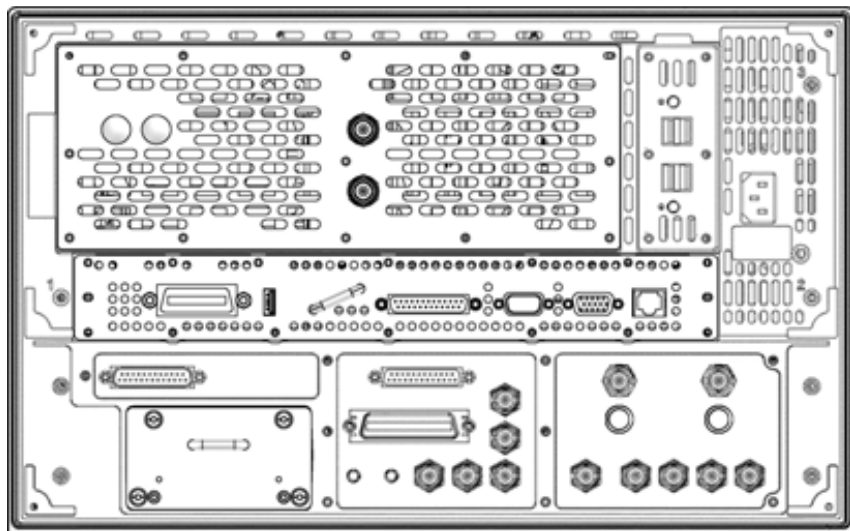

Powering the PNA ON and OFF

The following is described in this topic:

[How to...](#)

[Hibernate](#)

[ON](#)

[Shutdown](#)

[Turn OFF Autostart](#)

Note: If the PNA front-panel keypad or USB ports are not responding, SHUTDOWN or RESTART the PNA; do NOT Hibernate. This causes the PNA drivers to awaken from hibernation in the same corrupt state.

How to Log off, Shut down, Restart, or Hibernate the PNA.

WITH A MOUSE

1. On the PNA **System** menu, click **Windows Taskbar**
2. On the Windows Taskbar, click **Shutdown**
3. In the **What do you want the computer to do?** list, choose an action:
 - Log off (closes programs and disconnects from the network)
 - [Shut down](#)
 - Restart (shutdown and start)
 - [Hibernate](#)
4. Click **OK** to perform the action



WITHOUT A MOUSE

- To Hibernate, BRIEFLY press the [green power button](#).
- To Shutdown - ONLY if the PNA is locked and you cannot operate the mouse or keypad - Press and hold the power button for at least four seconds. **This practice should be avoided!** Repeated shutdowns in this manner WILL damage the hard drive. [Learn more about damaging the PNA hard drive.](#)
- **Recommended** - To SAFELY shutdown the PNA without a mouse, configure the PNA so you can choose what to do when the power button is briefly pressed (as in Step 3 above). PNAs shipped after June 2005 are already configured this way:
 1. From Windows Control Panel, select **Power Options**
 2. Click **Advanced Tab**
 3. Under **Power buttons**, select **Ask me what to do.**

4. Click **OK** to end configuration.

The next time the power button is pressed, a dialog box will ask **What do you want the computer to do?** Use the PNA front panel **Tab** and **Enter** keys to choose an action.

Hibernate Mode

- In hibernate mode the current instrument state is automatically saved to the hard disk before the PNA is powered OFF.
- When the PNA is powered ON, this instrument state is loaded, thus saving time over a full system boot-up.
- A password is NOT required to resume PNA operation after Hibernate mode.
- The hibernation state is the normal OFF state. A small amount of standby power is supplied to the PNA when it is in the hibernation mode. This standby power only supplies the power switch circuits and the 10 MHz reference oscillator; no other CPU-related circuits are powered during hibernation. To guarantee that your measurements meet the PNA specified performance, allow the PNA to **warm-up for 90 minutes** after the power button light has changed from yellow back to green.

ON Mode

- To turn ON the PNA press the yellow power button.
- The power button will change to green when power is ON.

Turn OFF PNA Autostart

The PNA application (835x.exe) always starts automatically when power is turned ON. To cause the PNA to NOT Autostart, do the following:

1. Minimize the PNA application.
2. From Windows Explorer, navigate to and double-click the following file: C:\Program Files\Agilent\Network Analyzer\Service\Toggle_PNA_Autostart.

The script toggles the PNA Autostart mode ON and OFF.

Shutdown Mode

- In shut down mode the current instrument state is NOT automatically saved before the PNA is powered OFF.
- When the PNA is again powered ON, a full system boot-up is performed and the PNA powers-up in the preset settings.
- A password is required to resume PNA operation after being in Shutdown mode.
- To guarantee that your measurements meet the PNA specified performance, allow the PNA to **warm-up for 90 minutes** after the power button light has changed from yellow back to green.

- The PNA should only be shut down for service or to provide security via password protection.
- The power button will change to yellow when power is OFF.

Note: If the PNA is locked and you cannot operate the mouse or keypad, shut down the PNA by pressing and holding the power button for at least four seconds.

This practice should be avoided! Repeated shutdowns in this manner WILL damage the hard drive. [Learn more about damaging the PNA hard drive.](#)

Unplugging the PNA

-
- Remove the power cord from the PNA ONLY when the power button is yellow, in either Hibernate or Shutdown mode.
If the power cord is removed while the power button is green (PNA ON), damage to the hard drive is **likely**.
 - The button will remain yellow for several seconds after the power cord has been removed.
 - When plugged back in and the power button is pressed to ON, the PNA starts in the mode it was in when the power cord was unplugged, either Hibernate or Shutdown.

Front Panel Interface

There are three ways to use the front panel keys:

- **Active Entry Toolbar** (quickest)
- **Launch Dialog Boxes**
- **Navigate Menus** (most comprehensive)


Other Quick Start topics

Active Entry Toolbar

Not all settings can be made this way. For making ALL settings use Menus.

You can make settings quickly using this four step procedure.


- (1) Press a key
- (2) View active entry
- (3) Select a function
- (4) Enter a value (if necessary)

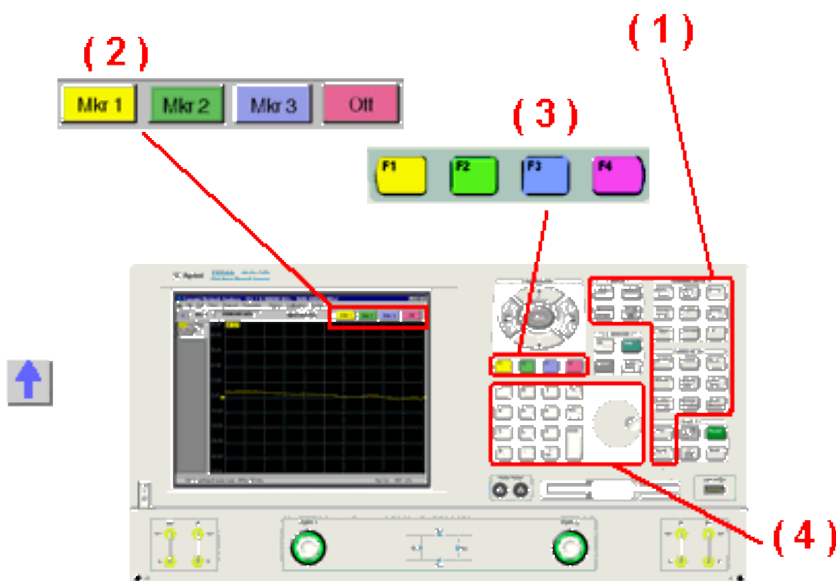

Launch Dialog Boxes,

To quickly launch MOST dialog boxes:


- (1) Press the Menu/Dialog Key
- (2) Select a function key

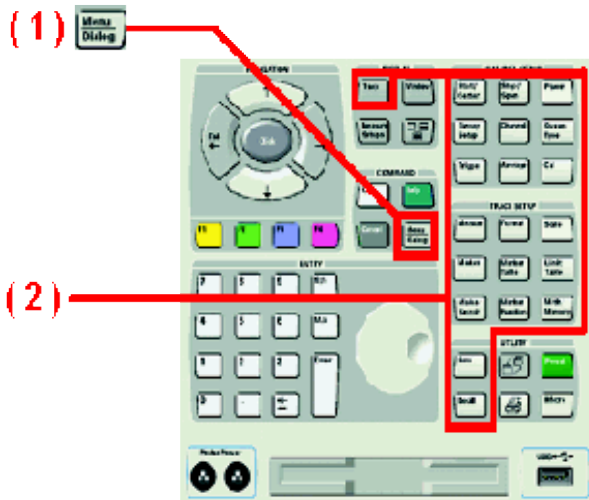

Navigate Menus

You can access ALL PNA functions using Menus:

- (1) Press the Menu/Dialog Key
- (2) Use the direction keys to navigate through the Menus. Use the "Click" key to make a selection.
- (3) Other Command keys are available for cancelling or seeking Help (if necessary)

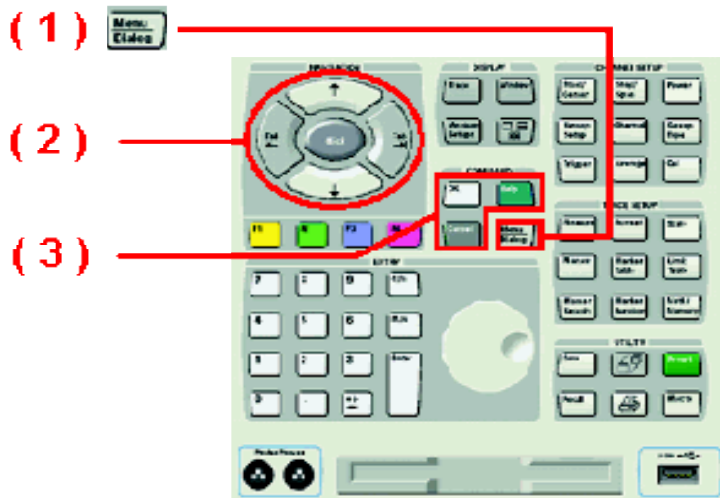

Traces, Channels, and Windows on the PNA

It is critical to understand the meaning of the following terms as they are used on the PNA.

Traces

Channels

Windows


Managing Windows

Note: You may experience a significant decrease in computer processing speed with combinations of the following: increased number of points, number of traces, and calibration error terms (full 2-port or 3-port). If this becomes a problem, you can increase the amount of RAM with PNA [Option 022](#). To monitor the amount of PNA memory usage, press **Ctrl Alt Delete**, select **Task Manager**, then click on the **Performance** tab.

Other Quick Start topics

Traces are a series of measured data points.

Trace settings affect the mathematical operations and presentation of the measured data. A trace must be selected (active) to modify its settings. To select a trace, click the [Trace Status](#) button. The following are Trace settings.

- Parameter
- Format
- Scale
- Calibration ON / OFF
- Trace Math
- Markers
-  • Electrical Delay
- Phase Offset
- Smoothing
- Transform

Channels contain traces. The PNA can have up to **32 independent channels**.

Channel settings determine **how** the trace data is measured . All traces that are assigned to a channel share the same channel settings. A channel must be selected (active) to modify its settings. To select a channel, click the [Trace Status](#) button of a Trace in that channel. The following are channel settings:


- Frequency span
- Power

- Calibration data
- IF Bandwidth
- Number of Points
- Sweep Settings
- Average
- Trigger (some settings)

Windows are used for viewing traces.

- The PNA can show up to **16 windows** on the screen.
- Each window can contain up to **8 traces** (4 traces previous to PNA release 5.2).
- Windows are completely independent of channels.
- Most Window settings are made from the **View** menu. See [Customize the PNA screen](#) for details.
- Learn to [create and manage windows](#).

The following is a window containing two traces. Both traces use the same channel 1 settings as indicated by the annotation at the bottom of the window.

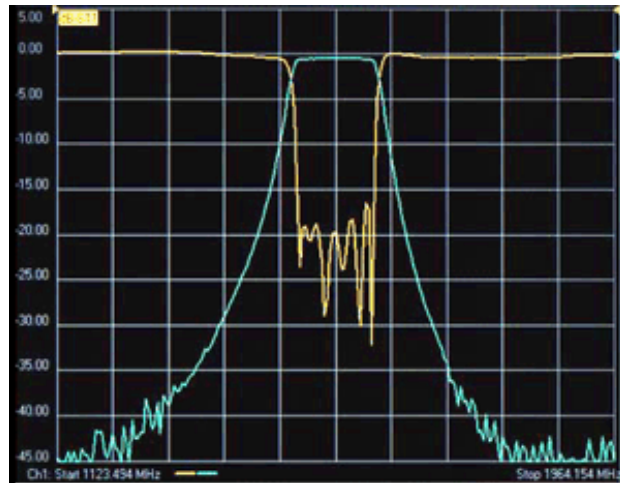

Managing Windows

How to create a new window

Use one of the following methods:

- Press  +    
- Click **Trace**, **New Trace**. Check **New Window**.
- Click **Window** then **New**. A new window appears with a default trace (S11, Ch1).


Learn more about using the [front panel interface](#)

How to view a window with the full screen view:

When more than four windows are on the screen, the Trace Status pane is hidden and resolution becomes poor. To view the window with the full screen:

Select the trace:

- Press  +    

Then press . Press again to minimize the window

Basic Measurement Sequence

The following process can be used to setup all PNA measurements:

Step 1. Set Up Measurements

Reset the analyzer, create a measurement state, and adjust the display.

Step 2. Optimize Measurements

Improve measurement accuracy and throughput using techniques and functions.

Step 3. Perform a Measurement Calibration

Reduce the measurement errors by performing a calibration.

Step 4. Analyze Data

Analyze the measurement results using markers, math operations, and limit tests.

Step 5. Print, Save or Recall Data

Save or print the measurement data.

Using Help

Help Rev. 2005-06-08
PNA Rev 5.25
N5230A 4-port ONLY
© Agilent Technologies, Inc. 2005

This topic discusses the following:

[Printing Help](#)

[Copying Help to your PC](#)

[Launching Help](#)

[Navigating Help](#)

[Help Languages](#)

[Glossary](#)

[Dialog Boxes](#)

[About Network Analyzer](#)

[Documentation Warranty](#)

[Suggestions Please](#)

Other Quick Start Topics

Printing Help

Beginning with the PNA 5.2 release (March 2005), we once again offer a .pdf version of PNA Help. Download the .pdf file from <http://www.agilent.com/find/pna>. Search for "PNA Help" and scroll to Manuals and Guides. You can still print individual PNA Help topics by clicking the Print icon at the top of the PNA Help window.



Copying Help to your PC

With the Help system on your PC, you can read about the PNA while away from it. You can also Copy and Paste programming code from this Help system directly into your programming environment.

The Help file is located on your PNA hard-drive at **C:\Winnt\Help\ PNAHelp.chm**. If both the PNA and PC are connected to LAN, you can [map a drive](#) and copy the file directly. The Help system can be downloaded from <http://www.agilent.com/find/pna>. Search for "PNA Online Help" and scroll to Manuals and Guides.

Launching Help

The Help system can be launched in three ways:


1. From the front panel [Help button](#).
2. From the **Help** drop-down menu

3. From Dialog Box Help

Navigating Help

The Help Window contains 3 panes (regions):

1. Toolbar Pane
2. Topic Pane
3. Navigation Pane

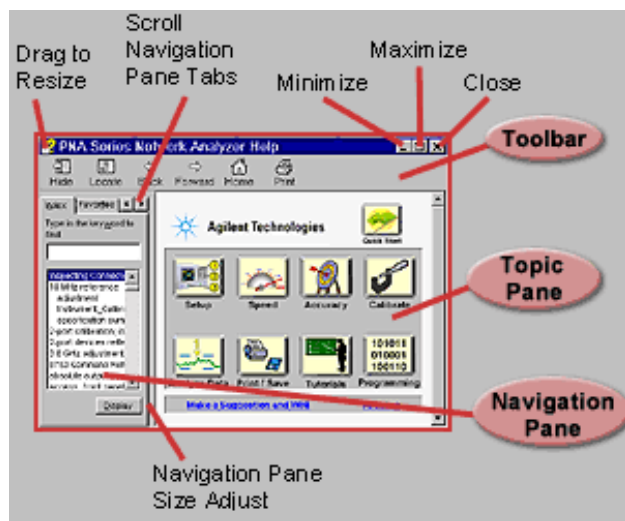

Toolbar Pane

The Toolbar is at the top of all Help windows. It allows you to resize the window, browse and print the selected topic.



1. Hide or show the navigation pane
2. Locate the topic in the table of contents
3. Back to topic visited previously
4. Forward again if **Back** was clicked
5. Go to the Home page.
6. Print the topic pane.

Navigation Pane

Click the following tabs in the Navigation Pane to access information in the Help system:


[Table of Contents Tab](#)

[Index Tab](#)

[Search Tab](#)

[Favorites Tab](#)


(Table of)Contents Tab

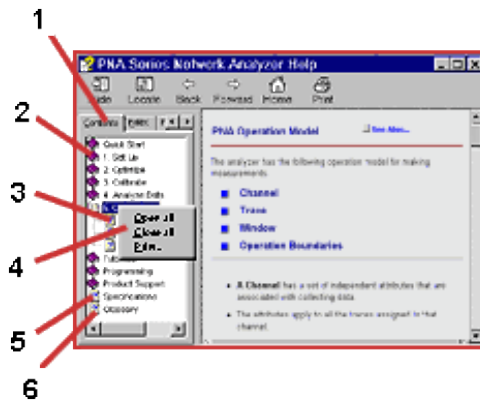

1. Click tab to select Table of Contents.
2. Click a book to access related topics.
3. Click to display a topic.
4. Right click to access menu.
5. Click to display specifications
6. Click to display glossary

Index Tab

The index tab allows you to type a keyword and go to only the most applicable topics.

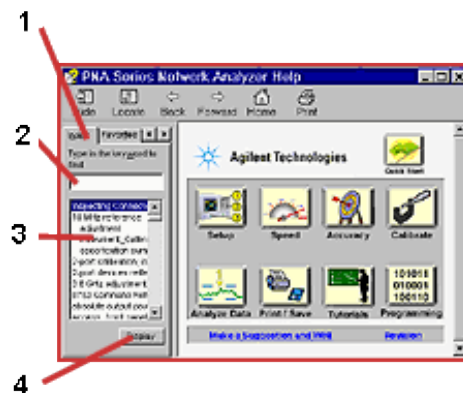

1. Click tab to select index.
2. Type keyword to find topics of interest.
3. View suggested topics. (Double-click to display topic.)
4. Click to display topic.

Search Tab


The following rules apply for using full-text search:

- Searches are not case-sensitive.
- You can search for any combination of letters (a-z) and numbers (0-9).
- Punctuation marks (period, colon, semicolon, comma, and hyphen) are ignored during a search.
- You can group the words of your search using double quotes or parentheses. Examples: "response calibration" or (response calibration). This requirement makes it impossible to search for quotation marks.
- Use Wildcard expressions:
 - To search for one undefined character use a question mark (?). For example, searching for **cal?** will find **calc** and **calf**.
 - To search for more than one undefined character use an asterisk (*). Searching for **Cal*** will find **calibration** and **calculate**.
- Use Boolean operators to define a relationship between two or more search words.

Search for	Example	Results will show topics containing:
Two words in the same topic	response AND calibration	Both the words "response" and "calibration".
Either of two words in a topic	response OR calibration	Either the word "response" or the word "calibration" or both.
The first word without the second word in a topic	response NOT calibration	The word "response" but not the word "calibration".
Both words in the same topic, close together.	response NEAR calibration	The word "response" within eight words of the word "calibration".

Favorites Tab

The favorites tab allows you to store (bookmark) the topics you refer to most often so that they can be recalled easily.

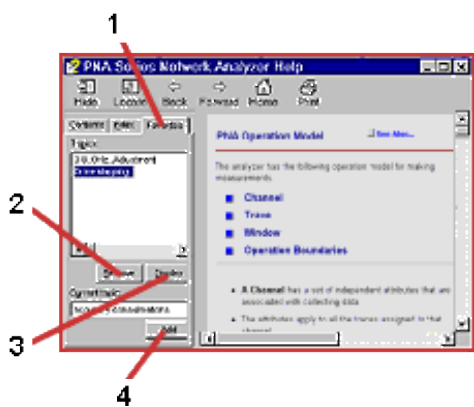


1. Click tab to view stored topics in Favorites.
2. Remove selected topic.

3. Display selected topic.
4. Add (store) current topic.

Topic Pane

The Topic pane allows you to view the contents of the selected topic.

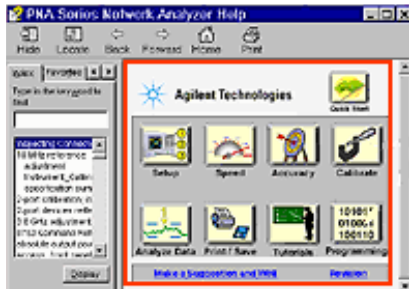

Help Languages

The Help system is available in five languages:

- English
- French
- German
- Japanese
- Spanish
- Chinese

To upgrade to the latest version, or to make Chinese Help available, use [AgileUpdate](#).

To select a different help language, on the **Help** menu, point to **Help Language**. Then click the language.

Note: The Programming and Specifications sections are only available in English. Also, the most recent version of Help will be English.

Viewing Help in Japanese or Chinese

These two languages use a different character font set than the other languages. To view these languages, you must change the following settings:

1. From the PNA, click **View**
2. Click **Title Bars** (if not already checked)
3. Minimize the PNA screen
4. From the desktop of the PNA, click **Start / Settings / Control Panel / Regional Options**.
5. Under **Language settings for the system**, scroll to and check **Japanese or Chinese**

6. Under **Your locale (location)** select **Japanese or Chinese**
7. Click **Set default...**
8. Under **Select the appropriate locale**, select **Japanese or Chinese**


These changes may cause the Windows 2000 fonts to become small. To change them back to larger fonts, change the following settings:

1. From the PNA desktop click **Start / Settings / Control Panel**
2. Click **Display / Appearance**
3. Under **Scheme** select **Windows Standard**

To restart the PNA application, click **PNA Analyzer** taskbar button at the bottom of the screen


Glossary

The Glossary holds definitions of words, in alphabetical order.

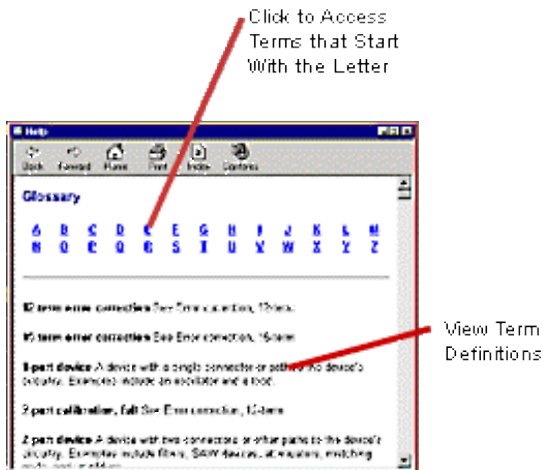

Note: Click on a word in green text throughout Help to see the glossary definition.

Dialog Boxes

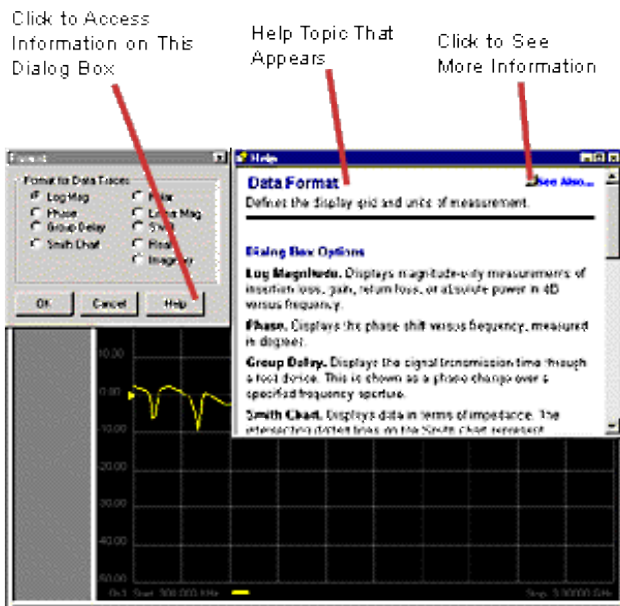

About Network Analyzer

To learn the following about your analyzer, click **Help**, then **About Network Analyzer**:

- Model number
- Frequency range
- Options installed on the analyzer
- Serial number of the analyzer
- Version of the installed analyzer software
- Version of hard drive in the analyzer

Documentation Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED "AS IS," AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, AGILENT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

AGILENT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD AGILENT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

Suggestions Please!

Please let us know about your experience using PNA Help. Send your comments to:

pna_help@am.exch.agilent.com. Comment about any aspect of the help system. Here are a few areas that you might consider:

- Does anything appear to be broken?
- Did you find what you were looking for?
- Was the information you found helpful?
- Any suggestions as to how we can improve the help system?

Your comments go directly to the help system authors. For help with technical questions, please refer to [Technical Support](#).

Preset the PNA

When you Preset the PNA, it is set to known, or preset conditions. You can use the factory default preset conditions, or define your own User Preset conditions.

[Preset \(Default\) Conditions](#)


[User Preset Conditions](#)

[See other 'Setup Measurements' topics](#)

Preset Default Conditions

How to Preset the PNA

Use one of the following methods:

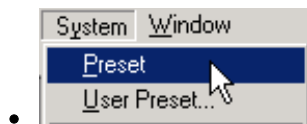

Learn more about using the [front panel interface](#)

Click to view the **factory preset conditions**.

[Frequency Settings](#)

[Power Settings](#)

[Sweep Settings](#)

[Segment Sweep Settings](#)

[Trigger Settings](#)

[Display Settings](#)

[Response Settings](#)

[Calibration Settings](#)

[Marker Settings](#)

[Limit Test Settings](#)

[Time Domain Settings \(Option 010\)](#)

[Global Display Settings](#)

Frequency Settings:

Measurement Parameter S11

Start Frequency Minimum frequency of the PNA

Stop Frequency Maximum frequency of the PNA

CW Frequency 1 GHz

See the [PNA configurations](#) for the minimum and maximum frequency of your PNA

Power Settings:

Test Port Power 0 dBm for E8356/7/8A
0 dBm for E8801/2/3A
0 dBm for N3381/2/3A

-5 dBm for N5230A - 20 GHz
-10 dBm for N5230 - 40 GHz
-15 dBm for N5230 - 50 GHz

-12 dBm for E8362/3/4 A or B, standard
-15 dBm for E8361A
-17 dBm for E8362/3/4 A or B with option UNL or 014

Port Power On
Coupled

Auto On
Attenuation

Attenuator 0 dB
Value

Power Slope Off

Slope Value 0 dB/GHz

Sweep Settings:

Type Linear Frequency

Mode Continuous

Generation Analog

Auto Sweep Time On

Number of Points 201

Segment Sweep Settings:

Active Segments 1

Start Frequency PNA start frequency

Stop Frequency 1 MHz for E8356/7/8A
1 MHz for E8801/2/3A
1 MHz for N3381/2/3A
1 GHz for E836xA/B

Number of Points 21

Power PNA preset test port power

IF Bandwidth 50 KHz for N5230A
35 kHz for all other models

Reduce IF BW at Low Frequencies ON

Dwell Time 0

Trigger Settings

Source Internal

Mode Sweep

Display Settings:

Format Log Mag

These settings apply for formats when selected:

Format	Scale	Reference Position	Reference Value
Log Mag	10 dB/	5	0 dB
Phase	45 degrees/	5	0 degrees
Group Delay	10 nsec/	5	0 s
Linear Mag	100 munits/	0	0 units
SWR	1 unit/	0	1 unit
Real	2 units/	5	0 units
Imaginary	2 units/	5	0 units
Polar	1 unit/	n/a	1 unit
Smith Chart	1 unit/	n/a	1 unit

Response Settings:

Channel Number	1
IF Bandwidth	50 KHz for N5230A 35 kHz for all other models
Averaging	Off
Averaging Factor	1
Smoothing	Off
Smoothing Factor	1% of span
Electrical Delay	0 s
Velocity Factor	1.0
Phase Offset	0 degrees
Math/Memory Trace View	Data

Calibration Settings:

Correction State	Off
Interpolation State	On
Calibration Type	None
Cal Kit Number	Current Cal Kit Number
System Z0	50 ohms
Port Extensions State	Off
Port Ext. Values	0
Input A, B	
Port 1, 2	

Marker Settings:

Initial Frequency	Current Center Frequency
Reference	None
Interpolation	On
Format	Trace Default
Type	Normal
Function	Max Value
Domain	Full Span
Table	Empty
Coupling	Always uncoupled

Limit Test Settings:

Limit Testing	Off
Line Display	ON
Sound on Fail	Off

Limit List Settings:

Type (OFF, MAX, MIN)	OFF
Begin Stimulus	0
End Stimulus	0
Begin Response	0
End Response	0

Time Domain Settings:

Transform State Off
Transform Mode Band Pass
Transform Start -10 ns
Transform Stop 10 ns
 Window 6.0 (Kaiser-Bessel factor)
Gating State Off
Gating Start -10 ns
Gating Stop 10 ns
 Gate Type Band Pass
 Gate Shape Normal


Global Display Settings:

Trace Status On
Frequency/ Stimulus Off
 Marker Readout On (when a marker is activated)
Toolbars Shown Active Entry
Status Bar State ON


User Preset Conditions

The analyzer can be **preset** to either **default** conditions or **User Preset** conditions.

How to set User Preset



Learn more about using the [front panel interface](#)

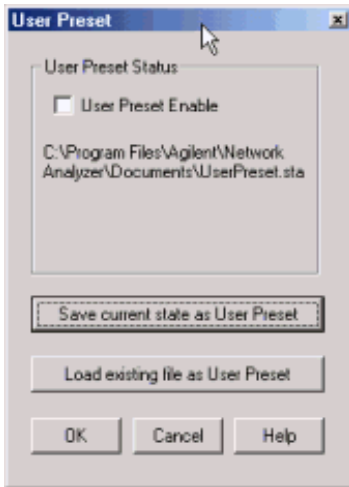

User Preset dialog box help

Allows the selection of User Preset conditions and the storing and recovery of those conditions.

User Preset Enable

Check - The PNA is preset to **User Preset** conditions when the Preset button is pressed.

Clear - The PNA is preset to **Default** conditions when the Preset button is pressed.

Save current state as User Preset Click to store the current instrument state as the User Preset conditions. File is stored as C:\Program Files\Agilent\Network Analyzer\Documents\UserPreset.sta.

Load existing file as User Preset Click to retrieve an instrument state to be used as the User Preset conditions.

Measurement Parameters

This topic contains the following information:

[S-Parameters](#) (pre-selected ratios)

[Ratioed](#) (choose your own ratio)

[Unratioed Power](#) (absolute power)

[How to Select a Measurement Parameter](#)

[Learn about Balanced Measurements](#)

[See other 'Setup Measurements' topics](#)

S-Parameters


S-parameters (scattering parameters) are used to describe the way a device modifies a signal. For a 2-port device, there are **four S-Parameters**. The syntax for each parameter is described by the following:

S out - in

out = port number where the signal output is measured (receiver)

in = port number where the signal is applied (source)

Move the mouse over each S-parameter to see the signal flow:

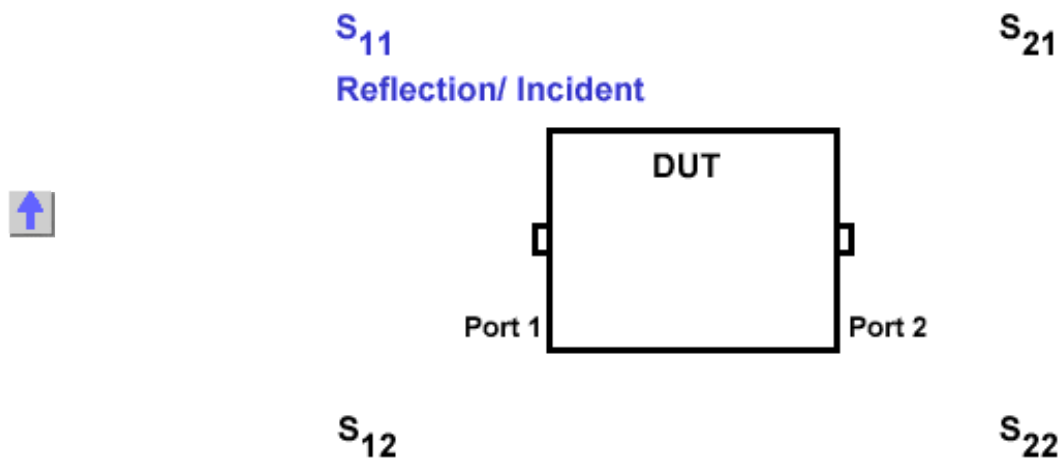

For two-port devices:

- When the source goes into port 1, the measurement is said to be in the **forward** direction.
- When the source goes into port 2, the measurement is said to be in the **reverse** direction.

The analyzer automatically switches the source and receiver to make a forward or reverse measurement. Therefore, the analyzer can measure all four S-parameters for a two-port device with a single connection.

See the [block diagram](#) (including receivers) of your PNA.

Common Measurements with S-Parameters

Reflection Measurements (S11 and S22)

- Return loss
- Standing wave ratio (SWR)
- Reflection coefficient
- [Impedance](#)
- S₁₁, S₂₂

Transmission Measurements (S21 and S12)

- [Insertion loss](#)
- Transmission coefficient
- Gain/Loss
- Group delay
- Deviation from linear [phase](#)
- [Electrical delay](#)
- S₂₁, S₁₂

Ratioed Measurements

Ratioed measurements allow you to choose your own ratio of input and reference signals using the receivers that are available in your PNA. Typically these are A, B, R1 and R2 receivers. S-parameters are actually predefined ratio measurements. For example S11 is A/R1.

The following are common uses of arbitrary ratio:

- Comparing the phase between two paths of a device. An example could be something simple like a power splitter or more complicated like a dual-channel receiver.
- Measurements that require a higher [dynamic range](#) than the analyzer provides with S-parameters.

See the [block diagram](#) (including receivers) of your PNA.

Your PNA **MAY** have front-panel jumper cables that go directly to measurement receivers. Learn about the [front-panel jumpers](#) on your PNA.


Unratioed Power

The unratioed power parameter allows you to look at the absolute power going into any of the measurement receivers that are available on your PNA.

Note: [Averaging for Unratioed parameters](#) is computed differently from ratioed parameters.

How to select a Measurement Parameter


Create a **NEW Trace** using either of the following methods:




OR



Change the **Active Trace** using either of the following methods:

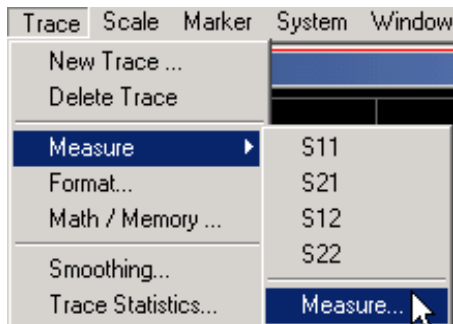


OR




Then click a tab to select the **TYPE** of measurement:


S-Parameters

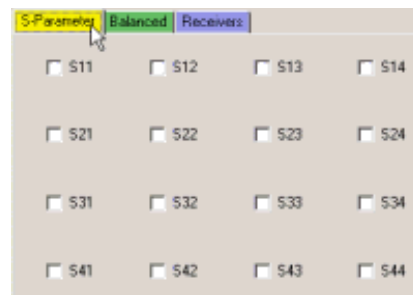

Balanced

Different measurements are available depending on the selected topology.

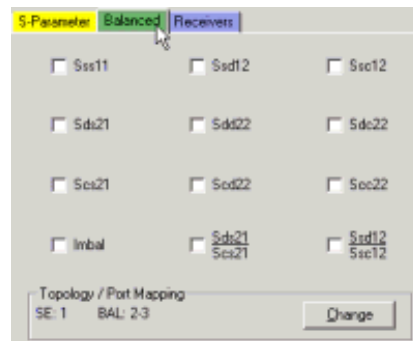


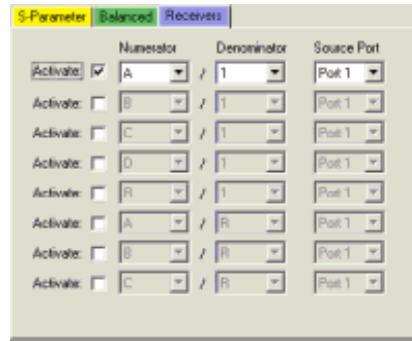

Receivers

- Ratioed
- Unratioed

Channel /
Window
Selections

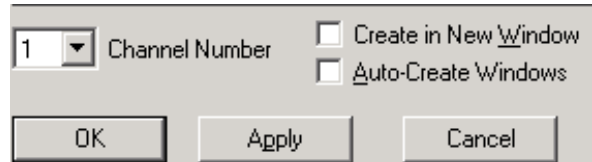

New Measurement - S-Parameters dialog box help

Click a tab to create or change measurements.

- When creating NEW measurements, you can choose more than one.
- When changing an EXISTING measurement, you can choose ONLY one.

Tabs

- **S-Parameters** Select a predefined ratioed measurements.
[Learn more about S-parameters.](#)
- **Balanced** Select a balanced measurement type. (4 port PNAs ONLY)
[Learn more about Balanced Measurements.](#)
 - [Change Topology / Port mappings](#)
- **Ratioed** Check Activate to create/change a measurement. Then select a receiver for the Numerator, select another receiver for the Denominator, then select a Source Port. For convenience, the table is populated with common choices.
[Learn more about Ratioed Measurements.](#)
See the [block diagram](#) of receivers in YOUR PNA.
- **Unratioed** Same as Ratioed, but select 1 as the Denominator.
[Learn More about Unratioed Measurements.](#)

Channel / Window Selections

These selections are NOT AVAILABLE when changing an EXISTING measurement. [Learn how to change a measurement.](#)

Channel Number Select the channel for the new traces.


Create in New Window

- Check to create new traces in a new window.

- Clear to create new traces in the active window. When the PNA traces per window limitation has been reached, no more traces are added.

Auto-Create Windows Check to create new traces in as many windows as necessary. See PNA number of windows limitation.

About Measurement Parameters (top of page)

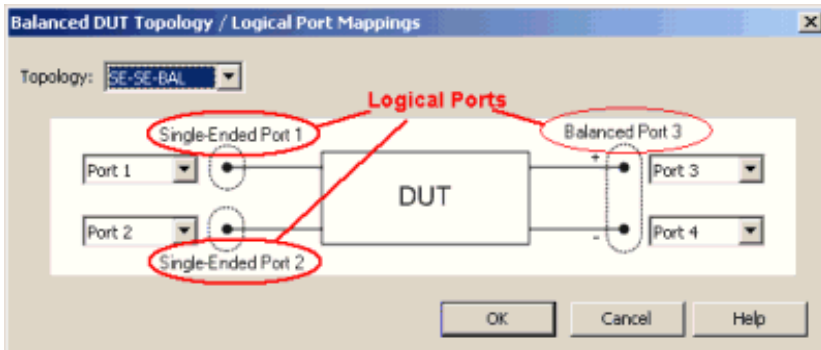

Balanced DUT Topology / Logical Port mappings dialog box help

Create or edit DUT Topology and Logical Port Mapping.

Note: These selections apply to ALL measurements in the channel. If the device topology is changed, any existing measurements in the channel that are incompatible with the new topology will be automatically changed to one that is compatible.

Topology: Describes your DUT as you would like it tested. The following device topologies can be measured by a 3-port or 4-port PNA.

- **Balanced / Balanced**
(2 logical ports - <4 actual ports>)
- **Single-ended / Balanced**
(2 logical ports - <3 actual ports>)
- **Single-ended - Single-ended / Balanced**
(3 logical ports - <4 actual ports>)

These topologies can be used in the reverse (<==) direction to measure:

- **Balanced / Single-ended** topology
- **Balanced / Single-ended - Single-ended** topology

For example, to measure a **Balanced / Single-ended** topology, measure the S12 (reverse direction) of a **Single-ended / Balanced** topology.

A Logical Port is a term used to describe a virtual port that is mapped to one or two PNA test ports.

- **One** Balanced Logical port is mapped to any **Two** PNA ports.

- **One** Single-Ended Logical Port is mapped to any **One** PNA port.

Learn more about [Balanced Measurements](#)

Frequency Range

Frequency range is the span of frequencies you specify for making a device measurement.

[How to Set Frequency Range](#)

[GW Frequencies](#)

[Frequency Resolution](#)

[Phase Lock Lost Indicator](#)

[Frequency Band Crossings](#)

[See other 'Setup Measurements' topics](#)

How to set Frequency Range


There are two ways to set the frequency range:

- Specify the Start and Stop frequencies of the range.
- Specify the Center frequency and desired span of the range.

The following will accomplish both methods:




The following settings will open dialog boxes:



Learn more about using the [front panel interface](#)


See the [frequency ranges of all PNA models](#)

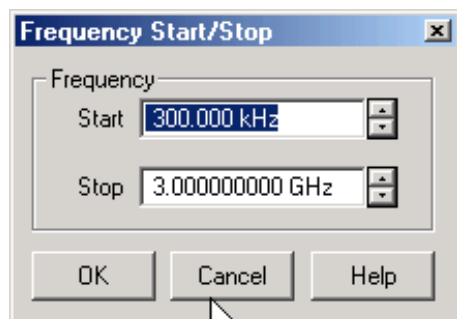

Frequency Start/Stop dialog box help

Start Specifies the beginning frequency of the swept measurement range.

Stop Specifies the end frequency of the swept measurement range.

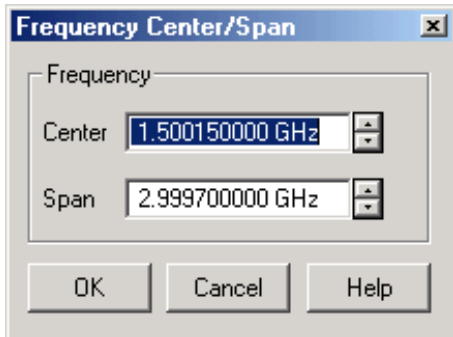

Frequency Center/Span dialog box help

Center Specifies the value at the center of the frequency sweep. This value can be anywhere in the analyzer range.

Span Specifies the span of frequency values measured to either side of the center frequency.

CW Frequencies


Measurements with a CW Time sweep or Power sweep as stimulus are made at a single frequency rather than over a range of frequencies.

How to set CW Frequency


First specify CW Sweep Type

You can set CW frequency from within the Sweep Type dialog box **or**

After specifying CW from the Sweep type dialog box, change CW frequency by selecting the following::



Learn more about using the front panel interface

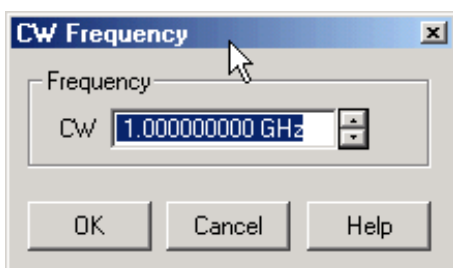

CW Frequency dialog box help

CW Type a value and the first letter of the suffix (k,m,or g) or use the up and down arrows to select any value within the range of the PNA.

Frequency Resolution

The resolution for setting frequency is 1 Hz.

Phase Lock Lost Indicator

Under normal operating conditions the analyzer stimulus frequency will be phase locked and within specifications ([see frequency specs](#)). If the analyzer is unable to create the stimulus frequency to specifications, a **Phase Lock Lost** message will appear on the screen ([see Troubleshoot the PNA](#)).

Frequency Band Crossings

The frequency range of the PNA covers several internal frequency bands. The higher the frequency range of the PNA, the larger the number of bands. The source power to your DUT turns off as the stimulus frequency is swept through these band crossings. To learn more, see [Power ON and OFF during Sweep and Retrace](#) and [Stimulus-Sweep Recommendation for a DUT with an AGC Loop](#).

Frequency band crossings are different for the following models:

- [3 GHz, 6 GHz, and 9 GHz Models](#)
- [E8362A/B, E8363A/B, E8364A/B](#)
- [E8361A](#)
- [N5230A \(2-port models\)](#)
- [N5230A \(4-port models\)](#)

For 3 GHz, 6 GHz, and 9 GHz PNA models:

Band	Frequency
1	10 MHz
2	748 MHz
3	1500 MHz
4	3000 MHz
5	4500 MHz
6	6500 MHz

For PNA models E8362 / 63 / 64 A/B
(A models do not have band 0)

Band	Freq (GHz)	Band	Freq (GHz)	Band	Freq (GHz)
0	.045				
1	0.748	9	7.60	17	25.60
2	1.500	10	10.00	18	30.00
3	3.00	11	12.00	19	32.00
4	3.80	12	12.8	20	36.00
5	4.50	13	15.20	21	38.40
6	4.80	14	16.00	22	40.00
7	6.00	15	20.00	23	45.60
8	6.40	16	22.80	24	48.00

For PNA model E8361A

Band	Freq (GHz)	Band	Freq (GHz)	Band	Freq (GHz)
0	.045	9	10.00	18	32.00
1	0.748	10	12.00	19	36.00
2	1.500	11	12.80	20	40.00
3	3.00	12	15.40	21	44.70
4	3.80	13	16.00	22	46.20
5	4.00	14	20.00	23	51.20
6	4.50	15	24.00	24	60.00
7	6.00	16	25.60	25	64.00
8	7.70	17	30.00		

For PNA model N5230A (2-port models)

Band	Freq (GHz)	Band	Freq (GHz)	Band	Freq (GHz)
1	.045	11	10.500	21	28.600
2	.748	12	12.500	22	31.250
3	1.5	13	15.750	23	31.500
4	3.125	14	16.667	24	33.333
5	4.167	15	18.750	25	37.000
6	5.250	16	21.000	26	40.500
7	6.250	17	22.500	27	41.667
8	7.875	18	25.000	28	42.000
9	8.333	19	26.250	29	46.800
10	9.375	20	26.500	30	

For PNA model N5230A Opt 240, 245 (4-port models)

Band	Freq (GHz)	Band	Freq (GHz)
0	.00112	9	8.333
1	0.010	10	9.800
2	0.040	11	10.500
3	0.748	12	12.500
4	1.500	13	15.000
5	3.125	14	15.750
6	4.166	15	16.666
7	5.250	16	18.750
8	6.250	17	20.100

Power Level

Power level is the power of the analyzer source signal at the test port. The following items describe details about power levels.

[Power Settings](#)

[Unleveled Indicator](#)

[Power Coupling Between Ports](#)

[Source Attenuation](#)

[Attenuation with Uncoupled Ports](#)

[Receiver Attenuation](#)

[Power Slope](#)

[Power ON and OFF during Sweep and Retrace](#)


[See other 'Setup Measurements' topics](#)

Power Settings

The test port output power is specified over frequency (See the [Power Range](#) and [Frequency Range](#) for your PNA)


How to make Power settings

Use one of the following methods:



Note: If Power Sweep is selected, (from [Sweep Type](#) dialog box) clicking **Channel, Power** will invoke a [Power \(Sweep\)](#) dialog box.

Learn more about using the [front panel interface](#)

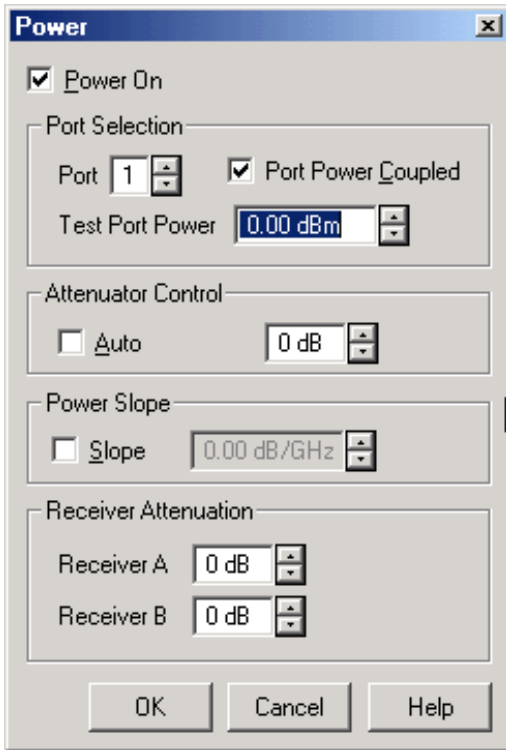

Power dialog box help

Defines and controls the analyzer source power.

Power On Toggles the source power ON and OFF.

Note: Power ON/OFF setting and Instrument State [Save and Recall](#).

If power is OFF when an instrument state is saved, the power will be OFF when the state is recalled.

If power is ON when an instrument state is saved, then when recalled, the power setting will be the SAME as the current power setting. To protect your DUT, power will NOT be turned ON by an instrument state recall if the current power setting is OFF.

Port Selection

Port Specifies the port which the values apply.

Port Power Coupled Toggles between coupled and uncoupled test port power. With the ports coupled, the power levels are the same at each test port. With the ports uncoupled, you can set different power levels for each test port. [Learn more about coupled ports.](#)

Test Port Power Sets the value of the power at the output of the test port.

Attenuator Control

This area of the dialog box is unavailable if there is no attenuator option installed in the PNA. If available, the value of attenuation placed in the source path can be chosen automatically or manually. If done manually, type or select an attenuation value in 10 dB increments. See [PNA Options](#) to view the availability and range of source attenuation on your PNA.

Auto Select to allow automatic attenuator control. The attenuation value select box will be unavailable. Clear to manually set the attenuator. Type or select the attenuation value in the adjacent text box.

Learn more about [Source Attenuation](#).

Power Slope

Compensates for a device's power loss over a frequency sweep by increasing the PNA output power over frequency.

Slope Select to set the power slope. Clear to set power slope OFF.

Learn more about [Power Slope](#).

Receiver Attenuation

Available on PNA models as [option 015](#) and [option 016](#).

Receiver A and **Receiver B** Type or select independent attenuation values for each receiver.

Learn more about [Receiver Attenuation](#).

Unleveled Indicator

The letters **LVL** appear on the status bar when the analyzer source is unleveled. To see the status bar, click **View**, then **Status Bar**.

LVL appears when the source power is **greater** than the maximum specified power. Resolve this by lowering the power level to return to a leveled condition (See your analyzer's [Power Range](#)).

If LVL continues to appear after lowering the source power, see [Troubleshoot the PNA](#) to determine the cause of the unleveled condition.

Power Coupling Between Ports

By default, the power level at each Port is **coupled to Port 1**. This means each Port will have the same output power level as Port 1. Some measurement applications require different power levels between ports. The analyzer allows you to **uncouple** the port powers so that you can set the power levels independently for each port.

For example, if you want to measure the gain and reverse-isolation of a high-gain amplifier, you must set the power for each port separately. This is because the power required for the input port of the amplifier is much lower than the power required for the output port. See [Attenuation With Uncoupled Ports](#).

CAUTION! You can damage the analyzer receivers if the input power levels exceed the maximum values. See your analyzer's [Technical Specifications](#) for the maximum input power to a receiver.

Source Attenuation

The PNA uses a programmable step source attenuator to cover the full power range. The attenuator adjusts the power level of the test signal into the test device without changing the level of the incident power in the reference path. This provides:

- Better signal source accuracy and performance
- A more accurate source match

Source attenuation is available on all PNAs in various ranges, either as standard equipment or as an option. If attenuation is not installed, the attenuator control is unavailable in the Power dialog box and not shown in the Active Entry Toolbar. See [PNA Options](#) to see the availability and range of source attenuation on your PNA.

The value of source attenuation can be set automatically or manually through the Power dialog box or front panel Power key.

Automatic Attenuation

With the attenuator control set to **Auto** (default), the analyzer:

- Allows you to select **any power level** within the total operating range of the instrument
- Automatically selects the attenuator position and source power so that the **optimum range** of the total attenuator range is used.

Manual Attenuation

There are some measurement applications where you need to set the source power and attenuator manually. These include:


- **Testing Reflection Amplifiers** (oscillators or conditionally unstable amplifiers). This requires a very good impedance match with the source (20dB return loss) over a wide frequency range. Choose **Auto Off**, with an attenuation level of 10 or 20 dB (or more) to ensure the best source match.
- **Power Sweeps** The attenuator is not allowed to switch attenuator settings during a power sweep to avoid premature wear from continuous switching. The Auto setting may not allow full coverage of the desired power sweep range. Choose **Auto Off** and a combination of source power range and attenuator position to provide the full desired power sweep range required for the measurement.

Attenuation Ranges and Values

The attenuator has different positions, allowing power levels in many power ranges. The number of power ranges available is determined by the source attenuation installed in your PNA. See [PNA Options](#) to see the availability and range of source attenuation on your PNA.

- Each range has a total specified span (25 dB in the following Attenuation Values graphic).
- The optimum setting is the middle of the range. This range provides the best accuracy and performance of the source leveling system. The optimum ranges are the blue regions in the following graphic.
- An attenuator setting can be selected manually or automatically. If automatic is selected, the blue optimum ranges (shown in the following graphic) are used.


(Attenuator ranges vary, this particular range is 70 dB)

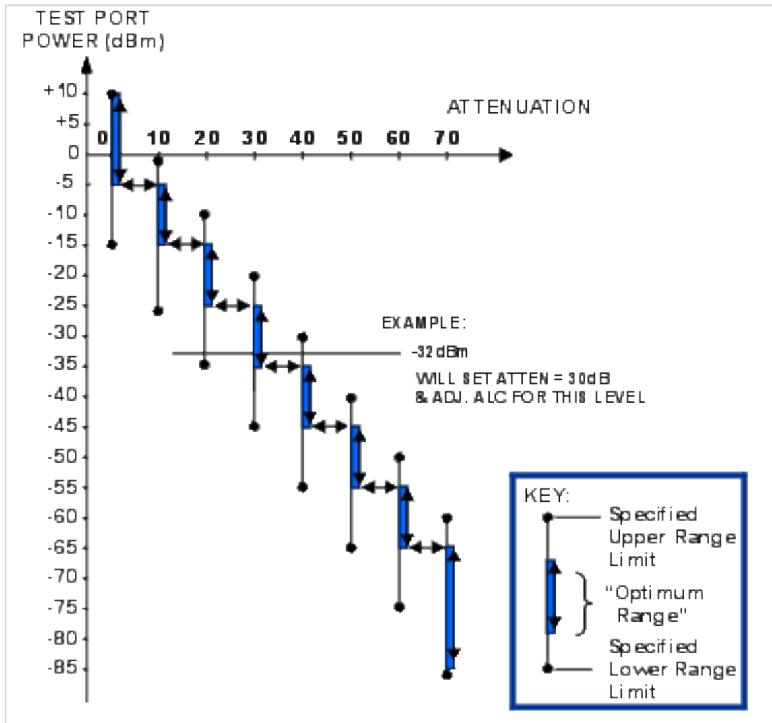

Note: Error correction is fully accurate only for the power level at which a measurement calibration was performed. However, when changing power within the same attenuator range at which the measurement calibration was performed, ratioed measurements can be made with nearly full accuracy (non-ratioed measurements with less accuracy).

Source Attenuation in Power Sweep

To set source attenuation in power sweep mode, first select Power Sweep type, then click **Channel, Power**

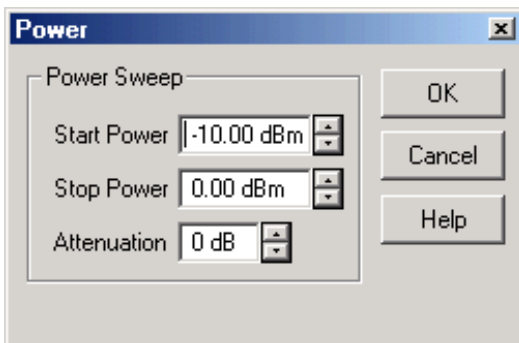

Power (Sweep) dialog box help

Start Power Sets the beginning value of the power sweep.

Stop Power Sets the end value of the power sweep.

Attenuation Sets the value of the source attenuator for both source ports.

[Learn more about Source Attenuation.](#)

[Learn more about Power Sweep.](#)

Attenuation with Uncoupled Ports

PNA models with Option UNL (and standard E8356/57/58A models) have a source attenuator with each test port. The test port power levels can be set independently.

PNA models with [Option 1E1](#) have a single source attenuator that is switched between test ports. If the ports are uncoupled, the test port power levels can be set differently. If the power levels are far apart, the single source attenuator will have to change position when switching between ports. To avoid premature wear of the mechanical step attenuator, the PNA does the following:

- Prevents continuous switching between power ranges
- Automatically engages hold mode after measuring each channel one time

If [averaging](#) is on, the hold mode does not engage until the specified number of sweeps is completed for each channel.

Receiver Attenuation

To avoid damaging the PNA receivers, you may need to attenuate the output signal from the device under test.

PNA models with [Option 015](#) or [Option 016](#) provide internal attenuators to both port receivers. The receiver attenuator characteristics are:

- Range:
 - 0 to 50 dB (E8361A only)
 - 0 to 35 dB (all other PNA models)
- Resolution:
 - 10 dB (E8361A only)
 - 5 dB (all other PNA models)

Power Slope

Power slope helps compensate for cable and test fixture power losses at increased frequency.

- With the power slope feature enabled, the port output power increases (or decreases) as the sweep frequency increases.
- The units of power slope are dB/GHz.
- Power slope can only be set to values of 0.5, 1, 1.5, or 2 (positive or negative).

Power ON and OFF during Sweep and Retrace

The frequency range of the PNA covers several internal frequency bands. The higher the frequency range of the PNA, the larger the number of bands. For example, a 9 GHz PNA has 6 frequency bands, a 50 GHz PNA has 25 frequency bands. See the [frequency band crossings](#).

Power to the DUT is set to minimum during band changes to avoid causing power spikes to the DUT. Minimum power is determined by the attenuator setting.

Retrace occurs when the source gets to the end of your selected frequency span and moves back to the start frequency. Power to the DUT is again set to minimum when retracing across frequency bands.

Therefore, the following occurs for various stimulus settings:

1. **Single band sweep** - The power to the DUT is always ON, even during retrace.
2. **Multi-band sweep** - The power to the DUT will go to minimum while sweeping across a band crossing. It will go to minimum again during retrace.
3. **Power sweep** - Because power sweep is always done at a single frequency, the frequency is always in a single band and the source power is always ON. At the end of a power sweep, power is immediately changed back to the start power. This helps prevent the DUT from overheating.
4. **Single sweep** - There are two methods of single sweep:
 - Manual trigger mode - At the end of a sweep the setup for the next sweep completes and the PNA waits for a trigger. During the setup of a multi-band sweep, the band swap completes and power to the DUT is turned back ON.
 - Hold mode - At the end of a sweep, power stays at minimum until the sweep is started.

Caution: Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

Sweep Settings

A sweep is a series of consecutive data point measurements taken over a specified sequence of stimulus values. You can make the following sweep settings:

[Sweep Type](#)

[Sweep Time](#)

[Sweep Setup](#)

See [Triggering and other 'Setup Measurements' topics](#)



Sweep Type

There are five sweep types in the PNA:


- **Linear Frequency** - Sets a linear frequency sweep that is displayed on a standard grid with ten equal horizontal divisions. This is the default sweep type.
- **Log Frequency** - Sets the source to step in logarithmic increments and the data is displayed on a logarithmic x-axis.
- **Power Sweep** - Activates a power sweep at a single frequency that you specify. You can set any power range < 25 dB. (Default -10 dBm to 0 dBm.) Power sweep is used to characterize power-sensitive circuits, with measurements such as gain compression or AGC (automatic gain control) slope. [Learn more about power sweep](#)
- **CW Time** - Sets the PNA to a single frequency, and the data is displayed versus time.
- **Segment Sweep** - Sets the PNA to sweep through up to 30 user-defined sweep segments. [Learn more about Segment sweep](#)

How to set Sweep Type

Use one of the following methods:

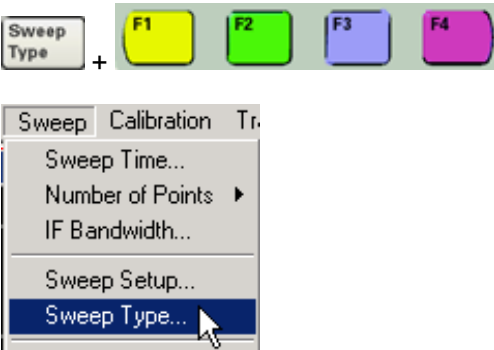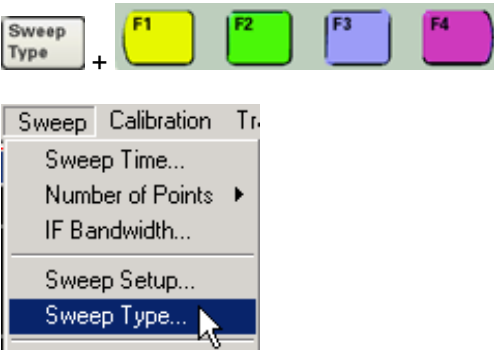- The image shows a screenshot of the front panel interface. At the top, there is a row of five buttons labeled F1 (yellow), F2 (green), F3 (blue), and F4 (purple). Below these is a 'Sweep Type' button. A dropdown menu is open from the 'Sweep Type' button, showing options: 'Sweep Time...', 'Number of Points' (with a right-pointing arrow), 'IF Bandwidth...', 'Sweep Setup...', and 'Sweep Type...' (which is highlighted with a mouse cursor).
• 

Learn more about using the [front panel interface](#)

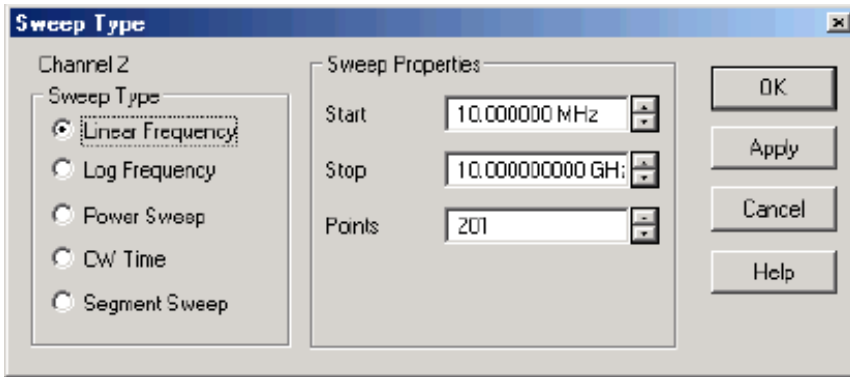

Sweep Type dialog box help

Note: Sweep Settings are not applied until either **OK** or **Apply** is pressed.

Channel The active channel when Sweep Type was selected. Sweep settings will be applied to this channel.

Sweep Type

Linear Frequency Sets a linear frequency sweep that is displayed on a standard grid with ten equal horizontal divisions.

- **Start** Sets the beginning value of the frequency sweep.
- **Stop** Sets the end value of the frequency sweep.
- **Points** Sets the number of data points that the PNA measures during a sweep. Range: 2 to 16001.(Default is 201).

Log Frequency The source is stepped in logarithmic increments and the data is displayed on a logarithmic x-axis. This is usually slower than a continuous sweep with the same number of points.

- **Start** Sets the beginning value of the frequency sweep.
- **Stop** Sets the end value of the frequency sweep.
- **Points** Sets the number of data points that the PNA measures during a sweep. Range: 2 to 16001. (Default is 201).

Power Sweep Activates a power sweep at a single frequency that you specify. [Learn about power sweep](#)

- **Start** Sets the beginning value of the power sweep.
- **Stop** Sets the end value of the power sweep.
- **CW Frequency** Sets the single frequency where the PNA remains during the measurement sweep.

CW Time Sets the PNA to a single frequency, and the data is displayed versus time.

- **CW Frequency** Sets the frequency where the PNA remains during the measurement.
- **Sweep Time** Sets the duration of the measurement, which is displayed on the X-axis.
- **Points** Sets the number of data points that the PNA measures during a sweep. Range: 2 to 16001.(Default is 201).

Segment Sweep Sets the PNA to sweep through user-defined sweep segments. [Learn how to make these settings.](#)

- **Independent Power Levels** Check to set the source power level for each segment. [Test port uncoupling](#) is also allowed.
- **Independent IF Bandwidth** Check to set the IF bandwidth for each segment.
- **Independent Sweep Time** Check to set the duration of the measurement for each segment.
- **X-Axis Point Spacing** Check to scale the X-Axis to include only the segments. [Learn more.](#)
- **Allow Arbitrary Segments** Check to allow arbitrary frequencies (overlapped or reverse sweeps). [Learn more](#)
- **Show Table** Shows the table that allows you to create and edit segments.
- **Hide Table** Hides the segment table from the screen.

OK Applies setting changes and closes the dialog box.

Apply Applies setting changes and leaves the dialog box open to make more setting changes.

Cancel Closes the dialog. Setting changes that have been made since the last Apply button click are NOT applied.

Power Sweep

Activates a power sweep at a single frequency that you specify. You can set any power range < 25 dB. (Default -10 dBm to 0 dBm.) Power sweep is used to characterize power-sensitive circuits, with measurements such as gain compression or AGC (automatic gain control) slope.

- Power is stepped from a start value to a stop value at a single frequency.
 - The source amplitude increases in discrete power steps at each data point across the power sweep range.
 - The number of data points and power range determine the size of these steps.
- Choose a combination of source power range and manual attenuator position (if the PNA has source attenuators) to obtain the power sweep range required for the measurement.

Note: To set the attenuation in power sweep, click **Channel, Power** after selecting Power Sweep.

In Power Sweep mode, the following power settings apply:

- Port Power Coupled setting (ON/ OFF) is ignored. Both test ports use the same Power Sweep settings.
- Test Port Power setting is ignored. The code uses the Start Power and Stop Power to determine the power levels present at the test ports.
- Attenuator Control is set to Manual
- Power Slope (dB/GHz) is ignored. The output frequency is CW.

Learn more about [Power Settings](#).

Segment Sweep

Segment Sweep activates a sweep which consists of frequency sub-sweeps, called segments. For each segment you can define independent power levels, IF bandwidth, and sweep time.

Once a measurement calibration is performed on the entire sweep or across all segments, you can make calibrated measurements for one or more segments.

In segment sweep type, the analyzer does the following:


- Sorts all the defined segments in order of increasing frequency
- Measures each point
- Displays a single trace that is a composite of all data taken

Restrictions for segment sweep:

- The frequency range of a segment is not allowed to overlap the frequency range of any other segment.
- The number of segments is limited only by the combined number of data points for all segments in a sweep.
- The combined number of data points for all segments in a sweep cannot exceed 16001.
- All segments are FORCED to have power levels within the same attenuator range to avoid premature wear of the mechanical step attenuator. See Power Level.

How to Insert, Delete, and Modify Segments

Insert and Delete Segments

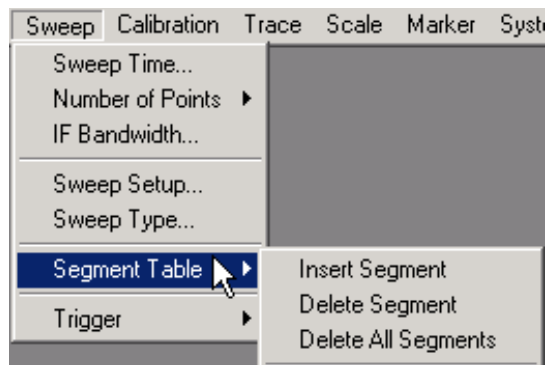

Insert Segment - adds a sweep segment before the selected segment.

Note- You can also click the "down" arrow on your keyboard to quickly add many segments.

Delete Segment - removes the selected segment

Delete All Segments - removes all segments

To Modify an Existing Segment

To make the following menu settings available, you must first show the segment table.

Click **View**, point to **Tables**, then click **Segment Table**.

	STATE	START	STOP	FOI	IFBW	P1 PwR	P2 PwR	TIME
1	ON	20.000000 MHz	1.000000 GHz	21	10.0 kHz	17.00 dBm	0.00 dBm	2.474 msec
2	ON	1.000000 GHz	4.000000 GHz	21	35.0 kHz	17.00 dBm	0.00 dBm	630.000 µsec

The above graphic shows the Segment table with all independent settings selected, including source power uncoupled (two power settings).

STATE Click the box on the segment to be modified. Then use the up / down arrow to turn the segment ON or OFF.

START Sets start frequency for the segment. Click the box and type a value and the first letter of a suffix (KHz, Mhz, GHz). Or double-click the box to select a value.

STOP Sets stop frequency for the segment. Click the box and type a value and the first letter of a suffix (KHz, Mhz, GHz). Or double-click the box to select a value.

POINTS Sets number of data points for this segment. Type a value or double-click the box to select a value.

To set IFBW, Power, and Sweep Time independently for each segment:

1. On the **Sweep** menu, click **Sweep Type**, then **Segment Sweep**.
2. Check the appropriate **Sweep Properties** boxes
3. Then click the box and type a value or double-click the box and select a value.

Note: If the following are NOT set, the entire sweep uses the channel IFBW, Power, and Time settings.

IFBW Sets the IF Bandwidth for the segment.

POWER Sets the Power level for the segment. You can also UNCOUPLE the test port power. See Power Coupling.

TIME Sets the Sweep time for the segment.

X-Axis Point Spacing

This feature applies to Segment Sweep only and affects how a trace is drawn on the screen.

How to select X-Axis Point Spacing

On the Sweep Type dialog box, click **Segment Sweep**

Then check **X-Axis Point Spacing**


Learn more about using the front panel interface

Without X-axis point spacing, a multi-segment sweep trace can sometimes result in squeezing many measurement points into a narrow portion of the x-axis.


With X-Axis Point Spacing, the x-axis position of each point is chosen so that all measurement points are evenly spaced along the x-axis.

For example, given the following two segments:

	STATE	START	STOP	POINTS
1	ON ▼	45.000000 MHz	50.000000 MHz	21
2	ON	170.000000 MHz	180.000000 MHz	21

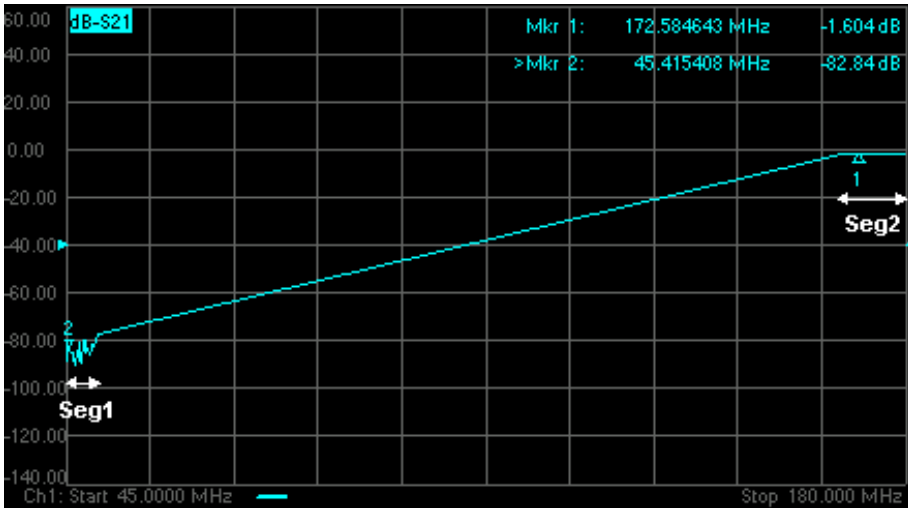

Without X-Axis Point Spacing

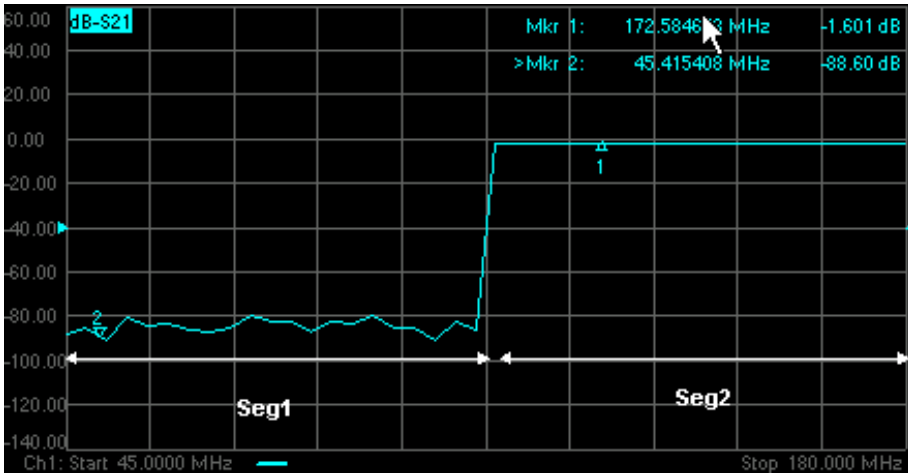

With X-Axis Point Spacing

Arbitrary Segment Sweep

This feature enables arbitrary frequencies to be entered into the segment sweep table, which allows the following:

- segments can have overlapping frequencies.
- reverse sweep (set the stop frequency to be less than the start frequency).

How to select Arbitrary Segment Sweep

On the Sweep Type dialog box, click **Segment Sweep**

Then check **Allow Arbitrary Segment Sweep**

Learn more about using the front panel interface

Note: The markers, display, limit lines, formatting, and calibration features may produce unusual results for overlapped and reverse sweep segments.

When Allow Arbitrary Segment is checked, X-axis point spacing is automatically turned ON.

Sweep Time


The PNA automatically maintains the fastest sweep time possible with the selected measurement settings. However, you can increase the sweep time.

How to set Sweep Time

Use one of the following methods:

- 
- 


Learn more about using the [front panel interface](#)

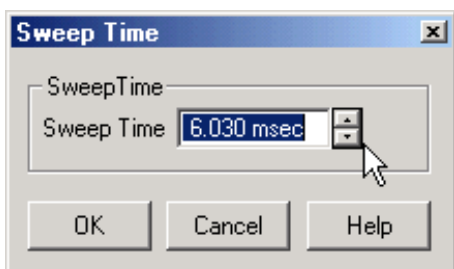

Sweep Time dialog box help

Specifies the time the PNA takes to acquire data for a sweep. The maximum sweep time of the PNA is 86400 seconds (1 day).


Note: If sweep time accuracy is critical, use ONLY the up and down arrows next to the sweep time entry box to select a value that has been calculated by the PNA. Do NOT type a sweep time value. For more details, refer to <http://na.tm.agilent.com/pna/accuracy.html>.

- The actual sweep time includes this acquisition time plus some "overhead" time.
- The PNA automatically maintains the fastest sweep time possible with the selected measurement settings. However, you can increase the sweep time using this setting.
- Enter **0** seconds to return the analyzer to the fastest possible sweep time.
- The Sweep Time setting is applied to the active channel.
- Stepped sweep is automatically selected if sweep time is at, or above, 8msec.
- A **Sweep Indicator**  appears on the data trace when the Sweep Time is 0.3 seconds or greater, or if trigger is set to Point Sweep Mode. The indicator is located on the last data point that was measured by the receiver. If the indicator is stopped (point sweep mode) the source has already stepped to the next data point.


Sweep Setup

How to make Sweep Setup settings

Use one of the following methods:

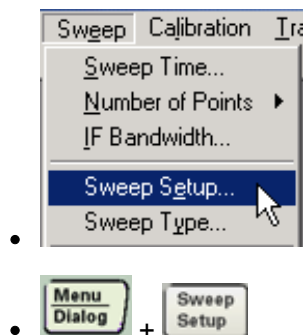

Learn more about using the [front panel interface](#)

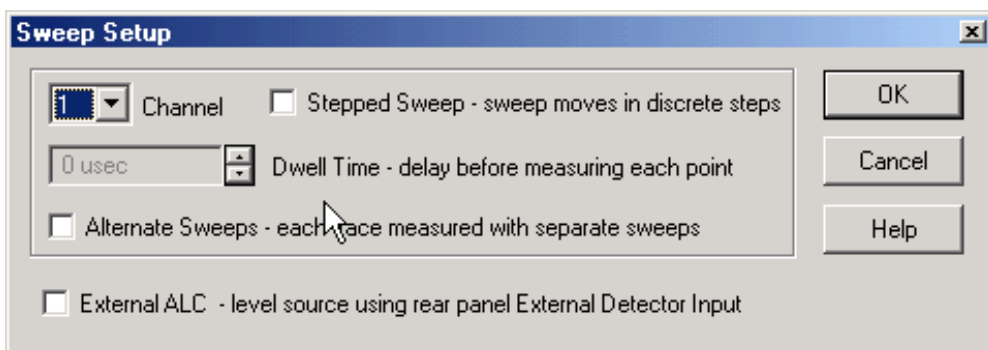

Sweep Setup dialog box help

Channel Specifies the channel that the settings apply to.

Stepped Sweep When checked (Stepped Sweep) the PNA source is tuned, then waits the specified Dwell time, then takes response data, then tunes the source to the next frequency point. This is slower than Analog Sweep, but is more accurate when testing electrically-long devices.

When cleared (Analog Sweep) the PNA takes response data AS the source is sweeping. The sweep time is faster than Stepped, but could cause measurement errors when testing electrically-long devices.

When the dialog checkbox is cleared, the PNA could be in either Analog or Step mode depending on the sweep time or IF bandwidth.

Stepped sweep is automatically selected when any of the following occur:

- IF Bandwidth is at, or below, 100Hz
- Sweep time is at, or above, 8msec.
- Source Power Correction is ON.

Dwell Time Specifies the time the source stays at each measurement point before the analyzer takes the data. Only applies to stepped sweep. The maximum dwell time is 100 seconds. See also [Electrically Long Devices](#).

Alternate Sweeps When checked, the PNA measures only one receiver per sweep. When cleared, the PNA measures both the A and B receivers (if used) each sweep. See also [Crosstalk](#).

External ALC When checked, the analyzer is enabled to receive an external signal that you provide for leveling the source output. The external ALC signal input connector is the External Detector Input on the rear panel. Available ONLY on 3 GHz, 6 GHz, and 9 GHz PNA models. Use this when using a booster amplifier in your test setup.

Trigger

A trigger is a signal that causes the PNA to make a measurement sweep. The PNA offers great flexibility in configuring the trigger function.

View the interactive [Trigger Model](#) animation to see how triggering works in the PNA.

[How to Set Trigger](#)

[Source](#)

[Scope](#)

[Channel Settings](#)


[Restart](#)

[External Triggering](#)

[See other 'Setup Measurements' topics](#)

How to Set Trigger

Use one of the following methods:

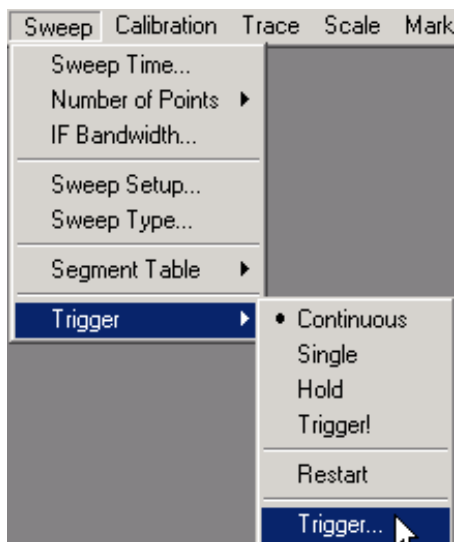


•



•

Learn more about using the [front panel interface](#)

Note: The settings Continuous, Single, Hold apply only to the active channel. These settings are available from the Sweep Trigger menu (shown above) and Active Entry keys.

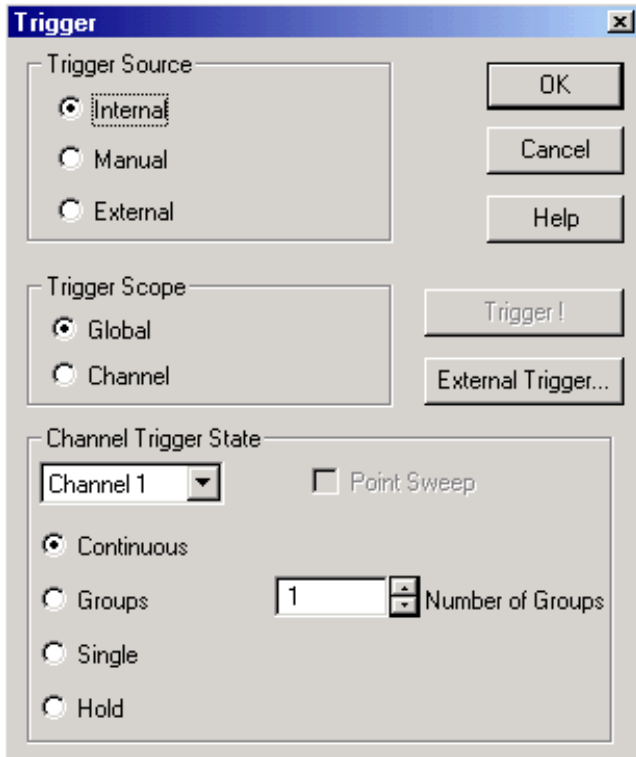

Trigger dialog box help

View the interactive [Trigger Model](#) animation to see how triggering works in the PNA.

Trigger Source

These settings determine **where** the trigger signals originate for all existing channels. A valid trigger signal can be generated only when the PNA is not sweeping.

Internal Continuous trigger signals are sent by the PNA as soon as the previous measurement is complete.

Manual One trigger signal is sent when invoked by the Trigger button, the active toolbar, or a programming command.

External Trigger signals are sent through the [Aux I/O connector \(pin19\)](#) on the rear panel. The trigger is level sensitive and can be either active TTL high or active TTL low.

Trigger Scope

These settings determine **what** is triggered.

Global All channels not in Hold receive the trigger signal [Default setting]

Channel Only the next channel that is not in Hold receives the trigger signal. This is not very obvious or useful unless Trigger Source is set to Manual. This setting enables Point Sweep mode.

Channel Trigger State

These settings determine **how many** trigger signals the channel will accept.

Note: When a trigger signal is received, ALL measurements in the channel are made; first the forward measurements (S11, S21) are made simultaneously - then reverse measurements (S12, S22). There are two exceptions to this:

1. When Alternate sweep is selected.
2. When Point Sweep is selected.

Continuous The channel accepts an infinite number of trigger signals.

Groups The channel accepts only the number of trigger signals that is specified in the Number of Groups text box, then goes into Hold. Before selecting groups you must first increment the Number of Groups text box to greater than one.

Number of Groups Specify the number of trigger signals the channel will accept before going into Hold. First increment to desired number, then select Groups.

Single The channel accepts ONE trigger signal, then goes into Hold.

Hold The channel accepts NO trigger signals.


Point Sweep When triggered, the channel measures the next data point in the sweep. Subsequent trigger signals go to the same channel until all of its measurements are complete. Then the next channel that is not in Hold is triggered. Available only when both Trigger Scope = CHANNEL and Trigger Source = MANUAL. See also the (point) Sweep Indicator.

Trigger! - Manually sends one trigger signal to the PNA.

External Trigger - Invokes the External Trigger dialog box.

Restart - Channels in Hold are set to single trigger (the channel accepts a single trigger signal). All other settings are unaffected, including decrementing trigger counts.

View the interactive Trigger Model animation to see how triggering works in the PNA.

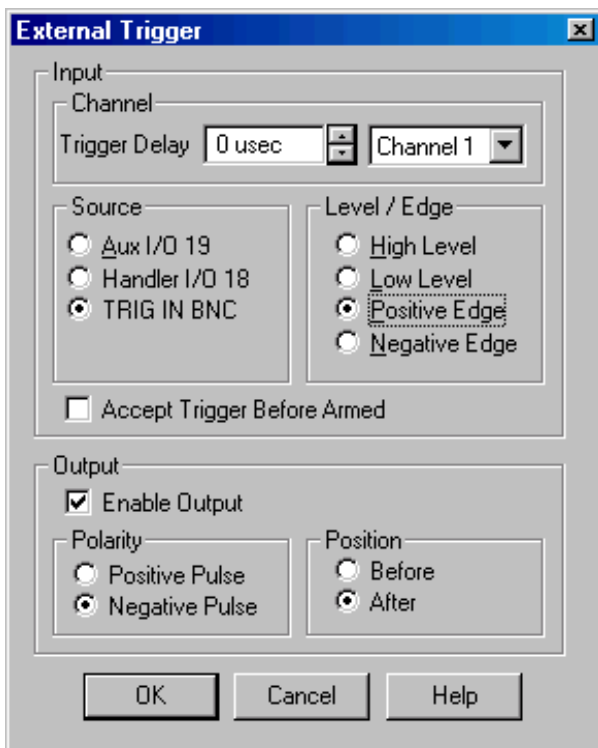

External Trigger dialog box help

Note: Although changes to settings in this dialog box affect the measurement immediately, you can click **Cancel** to revert to the previous settings.

Input

Trigger Delay After an external trigger is applied, the start of the sweep is held off for this specified amount of time plus any inherent latency.

Channel (Available only when Channel trigger is selected.) Select a channel to assume the specified trigger delay value. Each channel can have a different delay value.

Source The PNA accepts trigger input signals through one of the following input connectors:

- Aux I/O - pin 19
- Handler I/O - pin 18
- I/O 1 (TRIG IN) BNC

Level / Edge

High Level The PNA is triggered when it is armed (ready for trigger) and the TTL signal at the select input is HIGH.

Low Level The PNA is triggered when it is armed (ready for trigger) and the TTL signal at the select input is LOW.

Positive Edge After the PNA arms, it will trigger on the next positive edge. If Accept Trigger Before Armed is set, PNA will trigger as soon as it arms if a positive edge was received since the last data was taken.

Negative Edge After the PNA arms, it will trigger on the next negative edge. If Accept Trigger Before Armed is set, PNA will trigger as soon as it arms if a negative edge was received since the last data was taken.

Edge triggering is NOT available on the following PNA models: E835xA, E8362A, E8363A, E8364A.

Accept Trigger Before Armed When checked, as the PNA becomes armed (ready to be triggered), the PNA will immediately trigger if any triggers were received since the last taking of data. The PNA remembers only one trigger signal. All others are ignored.

When this checkbox is cleared, any trigger signal received before PNA is armed is ignored.

This feature is only available when positive or negative EDGE triggering is selected.

Output

Enable Output When checked, the PNA is enabled to send trigger signals out the rear-panel I/O (TRIG OUT) BNC connector.

Polarity The trigger pulse output from the PNA is either in the Positive or Negative direction.

Position The trigger pulse output is sent either BEFORE or AFTER a receiver measurement.

Configure external triggering remotely using CONTRol:SIGNal (SCPI) or ExternalTriggerConnectionBehavior (COM).

Data Format and Scale

A data format is the way the analyzer presents measurement data graphically. You should pick a data format appropriate to the information you want to learn about the test device.

[Rectangular \(Cartesian\) Display Formats](#)

[Polar](#)

[Smith Chart](#)

[How to Change Format](#)

[Scale, Reference Level and Position](#)

[Magnitude Offset](#)

[See other 'Setup Measurements' topics](#)

Rectangular Display Formats

Seven of the nine available data formats use a rectangular display to present your measurement data. This display is also known as Cartesian, X/Y, or rectilinear. The rectangular display is especially useful for clearly displaying frequency response information of your test device.

- Stimulus data (frequency, power, or time) appears on the X-axis, scaled linearly
- Measured data appears on the Y-Axis.

Log Mag (Logarithmic Magnitude) Format

- Displays Magnitude (no phase)
- Y-axis: dB



- Typical measurements:
 - Return Loss
 - Insertion Loss or Gain

Phase Format

- Displays Phase (no magnitude)
- Y-axis: Phase (degrees)
- Typical Measurements:
 - Deviation from Linear Phase

Group Delay Format

- Displays signal transmission (propagation) time through a device

- Y-axis: Time (seconds)
- Typical Measurements:
 - Group Delay

Linear Magnitude Format

- Displays positive values only
- Y-axis: Unitless (**U**) for ratioed measurements
Watts (**W**) for unratioed measurements.
- Typical Measurements:
 - reflection and transmission coefficients (magnitude)
 - time domain transfer

SWR Format

- Displays reflection measurement data calculated from the formula $(1+p)/(1-p)$ where p is reflection coefficient.
- Valid only for reflection measurements.
- Y axis: Unitless
- Typical Measurements:
 - SWR

Real Format

- Displays only the real (resistive) portion of the measured complex data.
- Can show both positive and negative values.
- Y axis: Unitless
- Typical Measurements:
 - time domain
 - auxiliary input voltage signal for service purposes

Imaginary Format


- Displays only the imaginary (reactive) portion of the measured data.
- Y - axis: Unitless
- Typical Measurements:
 - impedance for designing matching network

Polar Format

Polar format is used to view the magnitude and phase of the reflection coefficient (Γ) from your S11 or S22 measurement.

You can use Markers to display the following:

- Linear magnitude (in units) or log magnitude (in dB)
- Phase (in degrees)

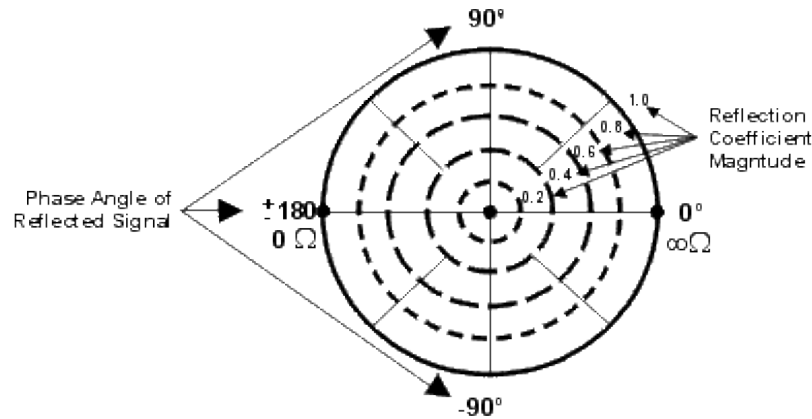

- The dashed circles represent reflection coefficient. The outermost circle represents a reflection coefficient (Γ) of 1, or total reflected signal. The center of the circle represents a reflection coefficient (Γ) of 0, or no reflected signal.
- The radial lines show the phase angle of reflected signal. The right-most position corresponds to zero phase angle, (that is, the reflected signal is at the same phase as the incident signal). Phase differences of 90° , $\pm 180^\circ$, and -90° correspond to the top, left-most, and bottom positions on the polar display, respectively.

Smith Chart Format



The Smith chart is a tool that maps the complex reflection coefficient (Γ) to the test device's impedance.

In a Smith chart, the rectilinear impedance plane is reshaped to form a circular grid, from which the series resistance and reactance can be read ($R + jX$).


You can use Markers to display the following:

- Resistance (in units of ohms)
- Reactance as an equivalent capacitance (in units of farads) or inductance (in units of henrys)


Rectilinear Impedance Plane



Smith Chart

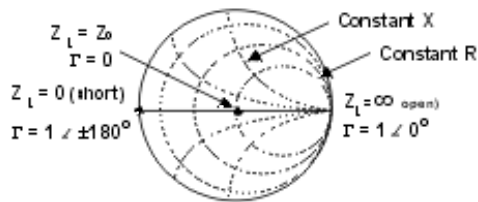

Interpreting the Smith Chart

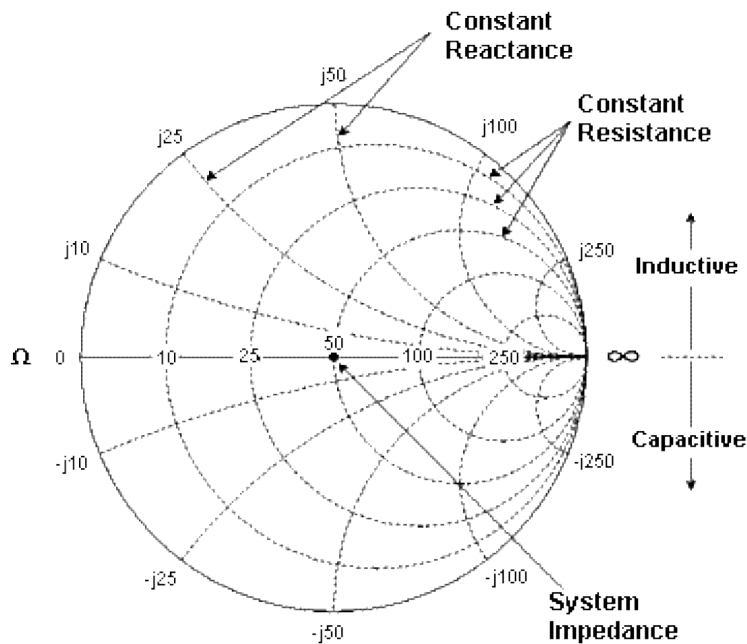





- Every point on the Smith Chart represents a complex impedance made up of a real resistance (r) and an imaginary reactance ($r+jX$)
- The horizontal axis (the solid line) is the real portion of the impedance - the resistance. The center of the horizontal axis always represents the system impedance. To the far right, the value is infinite ohms (open). To the far left, the value is zero ohms (short)

- The dashed circles that intersect the horizontal axis represent constant resistance.
- The dashed arcs that are tangent to the horizontal axis represent constant reactance.
- The upper half of the Smith chart is the area where the reactive component is positive and therefore inductive.
- The lower half is the area where the reactive component is negative and therefore capacitive.


How to set the Format

Use one of the following methods:



-  +    
-  + 

Learn more about using the [front panel interface](#)

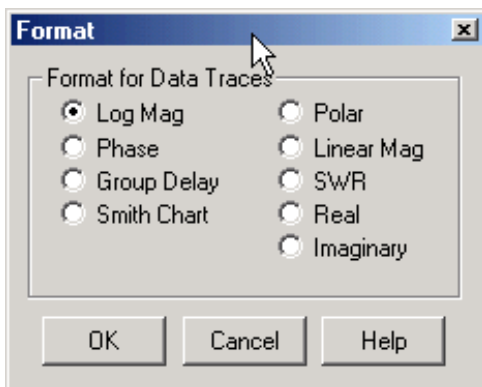

Format dialog box help

[Log Mag](#)

[Phase](#)

[Group Delay](#)

[Smith Chart](#)

[Polar](#)

[Linear Mag](#)

[SWR](#)

[Real](#)



[Imaginary](#)

Scale, Reference Level and Position


The Scale, Reference Level and Reference Position settings (along with format) determine how the data trace appears on the PNA screen.

How to set Scale, Reference Level, and Position

Use any of the following methods:

- 
- 

Learn more about using the [front panel interface](#)

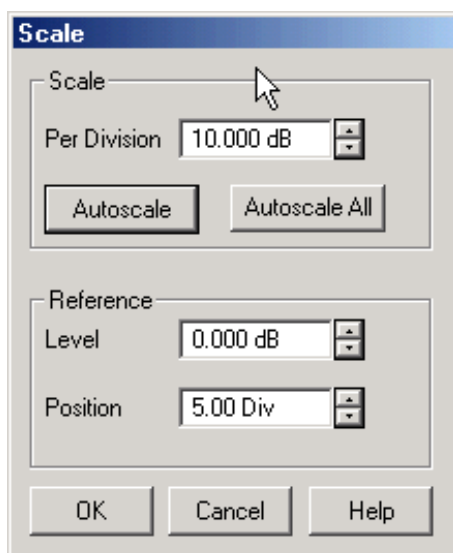

Scale dialog box help

Scale

Per Division Sets the value of the vertical divisions of a rectangular display format. In Polar and Smith Chart formats, scale sets the value of the outer circumference. Range: 0.001dB/div to 500 dB/div


Autoscale - Automatically sets value of the vertical divisions and reference value to fit the ACTIVE data trace within the grid area of the screen. The stimulus values and reference position are not affected.

The analyzer determines the smallest possible scale factor that will allow all the displayed data to fit onto 80 percent of the vertical grid.

The reference value is chosen to center the trace on the screen.

Autoscale All Automatically scales ALL data traces in the ACTIVE WINDOW to fit vertically within the grid area of the screen.

Reference

Level In rectangular formats, sets the value of the reference line, denoted by  on the PNA screen. Range: -500 dB to 500 dB.

In Polar and Smith chart formats, reference level is not applicable.


Position In rectangular formats, sets the position of the reference line. Zero is the bottom line of the screen and ten is the top line. Default position is five (middle).

In Polar and Smith chart formats, reference position is not applicable.

Magnitude Offset

Magnitude Offset allows you to offset the magnitude (not phase) data by a fixed and / or sloped value in dB. If the display format is Linear Magnitude or Real (unitless), the conversion from dB is performed and the correct amount of offset is implemented.

How to set Magnitude Offset



Learn more about using the [front panel interface](#)



Magnitude Offset dialog box help

The Magnitude offset setting affects only the active trace.

Offset Offsets the entire data trace by the specified value.

Slope Offsets the data trace by a value that changes with frequency. The offset slope begins at 0 Hz.

For your convenience, the offset value at the start frequency is calculated and displayed.

See where this operation is performed in the [data processing chain](#).

Pre-configured Measurement Setups

Pre-configured setups for NEW measurements

Pre-configured arrangements for EXISTING measurements

Before reading this topic, it is important to understand [Traces, Channels, and Windows](#) in the PNA.


[See other 'Setup Measurements' topics](#)

Pre-configured Setups for NEW Measurements

Each of the following setups **creates new traces**. Existing traces and their settings will be lost, unless you first save them.

How to select a pre-configured measurement setup


Use one of the following methods:

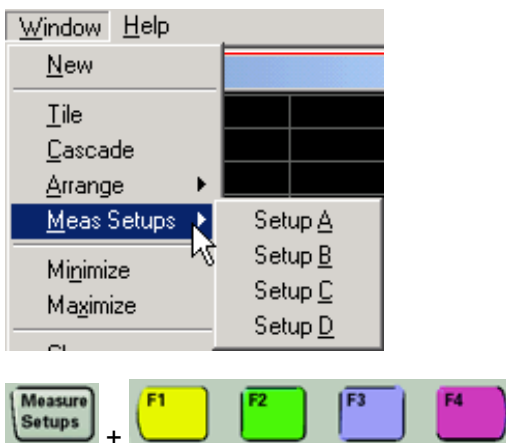

Learn more about using the [front panel interface](#)



The following are the four pre-configured measurement setups:

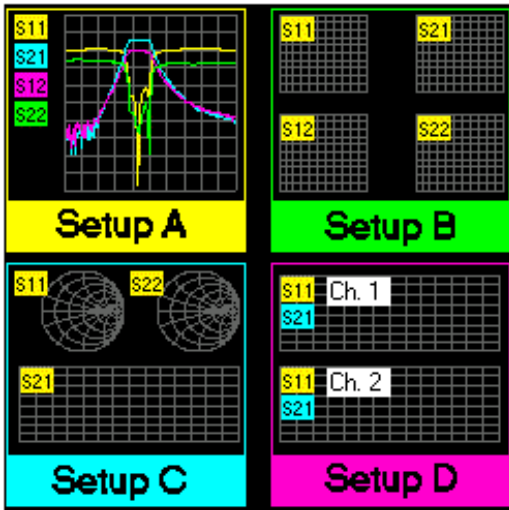


Arranging Existing Measurements


The following arrangements place EXISTING measurements into pre-configured Window arrangements using a sort algorithm.

How to select an Existing measurement arrangement

Use one of the following methods:

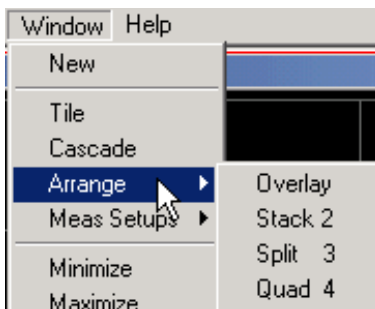

-




-

Learn more about using the [front panel interface](#)


Overlay Arrangement

This configuration places all existing traces in a single window, all overlaid on each other.

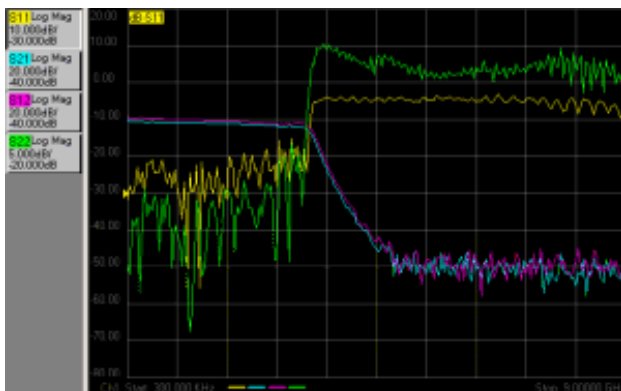


Stack 2 Arrangement

This configuration places all existing traces in two "stacked" windows.

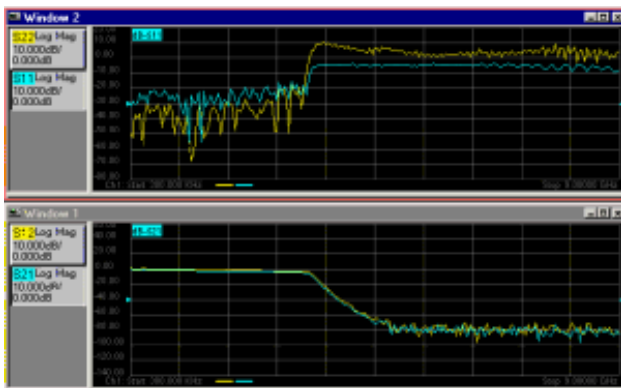


Split 3 Arrangement

This configuration places all existing traces in three windows, two on top and one below.

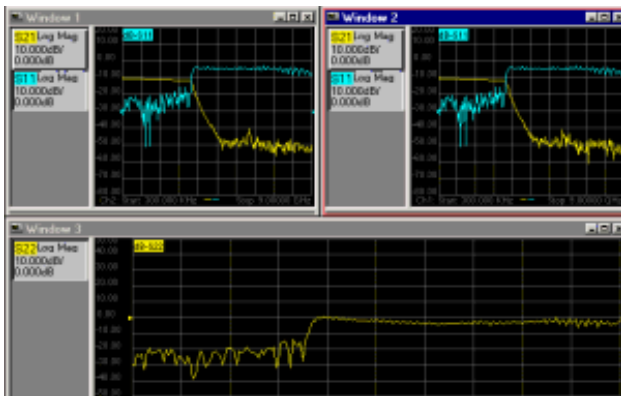

Quad 4 Arrangement

This configuration places all existing traces in four windows, one window in each screen quadrant.

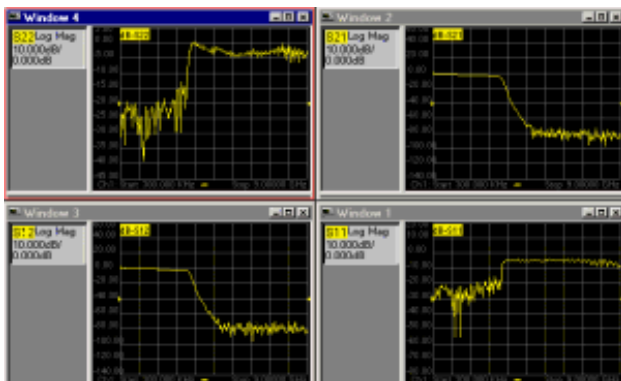

Sort Algorithm

The sort algorithm for the Arrange Windows feature is designed to:

- Divide traces among windows based on their properties
- Group traces with common properties

The algorithm sorting is based on the following trace properties, in order of priority:

1. Format: circular (polar or Smith) versus rectilinear (log mag, lin mag, group delay, etc.)
2. Channel number
3. Transmission versus reflection

Note: The PNA traces per window limitation overrides this algorithm. An error occurs if the arrange selection cannot be completed with the current number of traces on the screen.

Customize the PNA Screen

You can customize your PNA screen by showing or hiding the following display elements. All of these selections are made from the PNA **View** menu.

Status Bar

Toolbars

Tables

Measurement Display

Data and Memory Trace

Title Bars

Minimize Application

Learn about using [pre-configured measurements and windows arrangements](#)


Learn about [Traces, Channels, and Windows on the PNA](#)

See other 'Setup Measurements' topics

Status Bar



When enabled, the status bar is displayed along the bottom of the PNA screen. The primary status bar shows the following:

- Active channel
- Measurement parameter for the active trace
- Trace Math
-  Error correction for the active trace
- Averaging Factor for the active channel
- Smoothing Percentage
- Transform (On)
- Gating (On)
- IF Gating Enabled for Pulsed App: (G)
- Manual IF Filtering for Pulsed App: (F)
- Delay if invoked using Phase Offset, Electrical Delay, or Port Extensions.
- Loss if invoked using Magnitude Offset or Port Extensions
- GPIB status: Local (LCL), Remote Talker Listener (RMT), or System Controller (CTL).

- Error Status: (LVL, LCK, etc)

Note: A second level status bar appears when using Interface control or E5091 Testset control.

The status bar state (ON or OFF) will not change when the PNA is Preset.

How to display the Status bar




Learn more about using the [front panel interface](#)

Toolbars

You can display up to five different toolbars to allow you to easily set up and modify measurements.

How to display toolbars

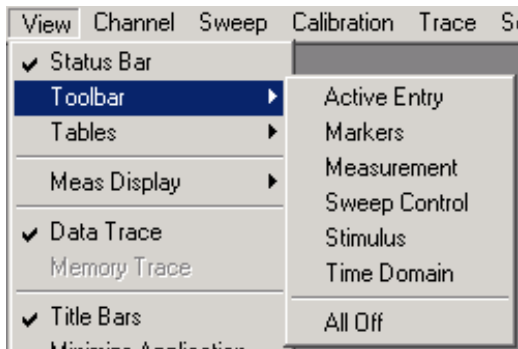

Learn more about using the [front panel interface](#)

Learn about each toolbar:

[Active Entry](#)

[Markers](#)

[Measurement](#)

[Sweep Control](#)

[Stimulus](#)

[Time Domain](#)

[Port Extension](#)

[All Off](#)

Note: There is also a Cal Set toolbar available for Monitoring Error Terms.


Active Entry Toolbar



The active entry toolbar is displayed at the top of the screen, below the menu bar. It allows you to make selections

from the active function using the mouse or by pressing the front panel key with the corresponding color.
Learn more about using the [front panel interface](#)

Markers Toolbar



The markers toolbar allows you to set up and modify markers. It shows:

- Marker number
- Stimulation value
- Marker functions
 - Delta
 - Start/Stop
 - Center/Span

Tip: To use the [Front Panel Knob](#) to change marker position, first click the **Stimulus** field of the marker toolbar. Then turn the knob.

[Learn more about Markers](#)

Measurement Toolbar



The measurement toolbar allows you to **create a new trace** for a desired S-parameter measurement in a current window or new window.

Sweep Control Toolbar



In left to right order, the buttons on this toolbar set the active channel to:

- **Hold** mode
- **Single** sweep, then Hold mode
- **Continuous** sweep

Learn more about [Channel Trigger State](#).


Stimulus Toolbar



The stimulus toolbar allows you to view, set up, and modify the sweep stimulus. It shows the:

- **Start** value
- **Stop** value
- Number of **points**

Time Domain



The Time Domain toolbar allows you to do the following:

- Turn Transform and Gating ON / OFF
- Change the Start / Stop times for both Transform and Gating
- **More...** launches the Time Domain Transform dialog box
- **X** Closes the toolbar

The front panel Tab key steps through all of the settings on all of the toolbars on the display. If Tab does not work, press one of the Active Toolbar (color) keys.

Port Extension



The Port Extension toolbar allows you to set Port Extensions while viewing the measurement trace. Learn more about Port Extensions.


All Off

This allows you to **hide all toolbars** with a single selection.

Tables

Tables are displayed at the bottom of the selected window. Only one table may be displayed at a time for a window.

How to display Tables

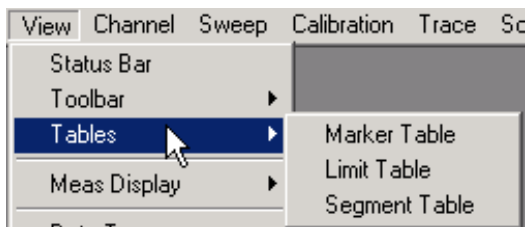

Learn more about using the front panel interface

You can display tables for the following:

Marker Table

Limit Line Table

Segment Table

Marker Table

You can display a table of marker settings. These settings include the:

- Marker number
- Marker reference (for delta measurements)
- Frequency

- Time and Distance (for Time Domain measurements)
- Response

Learn more about [Markers](#)

Limit Line Table

You can display, set up, and modify a table of limit test settings. These include:

- Type (MIN, MAX, or OFF)
- Beginning and ending stimulus values
- Beginning and ending response values

Learn more about [Limit Lines](#)

Segment Sweep Table


You can display, set up, and modify a table of segment sweep settings. These include:

- State (On/Off)
- Start and Stop frequencies
- Number of Points
- IF [Bandwidth](#) (if independent levels)
- Power Level (if independent levels)
- Sweep Time (if independent levels)

Learn more about [Segment sweep](#)

Measurement Display

How to display measurement information

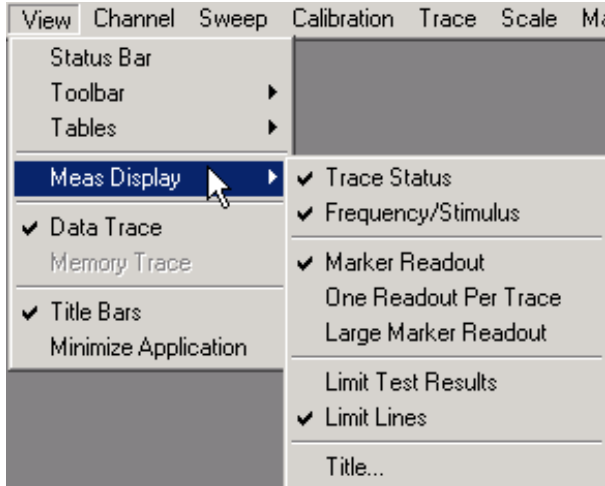

The screenshot shows a software menu titled 'View' with several sub-menus. The 'Meas Display' sub-menu is expanded, showing the following options:

- Trace Status (checked)
- Frequency/Stimulus (checked)
- Marker Readout (checked)
- One Readout Per Trace
- Large Marker Readout
- Limit Test Results
- Limit Lines (checked)
- Title...

Learn more about using the [front panel interface](#)

Trace Status

Frequency Stimulus

Marker Readout

Limit Test Results

Limit Lines

Title

Trace Status



Trace status is displayed to the left of each window on the screen. It shows the:

- Measurement parameter
- Format
- Scaling factor
- Reference level

Click a trace status button to make that measurement active.

How to display Trace Status buttons

Frequency/Stimulus

Ch1: Start 300.000 kHz ——— Stop 3.00000 GHz

Frequency/stimulus information is displayed at the bottom of each window on the screen. It shows:

- Channel number
- Start value
- Stop value

How to display Frequency/Stimulus information

Marker Readout

>Mkr 1: 1.500150 GHz -62.98 dB

- Checked - Shows the following marker information in the top right corner of each window.
 - Marker number
 - Stimulus value
 - Response value in marker's selected format
- Cleared - Shows **no** marker readout.

One Readout Per Trace

- Checked - Shows the readout of only the **active marker** for each trace.
- Cleared - Shows up to 5 marker readouts per trace, up to 20 total readouts.

Large Marker Readout

- Checked - Shows the marker readout in **large font size for easy reading**.
- Cleared - Shows the marker readout in **normal font size**.

Learn more about [Markers](#)

How to change Marker readout settings

Limit Line Test Results

Limit line test results, **Pass** or **Fail**, are displayed on the right side of the designated window.

Limit Lines

Limit lines are displayed for the active trace in the designated window. Their position depends on:


- Limit levels
- Format
- Scaling
- Reference level

Learn more about [Limit Lines](#)

How to display Limit Lines and Results

Title

You can create and display a title for each measurement window using the keyboard. You can also use the following Title Entry dialog box.

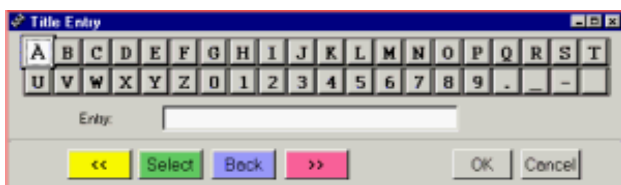

The title is displayed in the upper-left corner of the selected window.

To clear a title, delete the title from the dialog box entry area and click OK.

How to display a Title

Data Trace and Memory Trace

You can view or hide the active data or memory trace.

- Make a trace active by clicking the trace status button
- To view a memory trace you must first store a trace in memory. Click **Trace**, then **Math / Memory**, then **Data**

=> **Memory.**

Learn more about [Math operations](#)

Title Bars



The Title bar shows the window number and Minimize / Maximize icons.

Checked - Title bars for all PNA windows are shown.


Cleared - Title bars for all PNA windows are hidden. This allows more room to display measurement results.

How to change the Title Bar setting

Minimize Application

On the PNA Menu, Click View / Minimize Application to minimize the PNA application to the Windows taskbar.

To restore the PNA application:

- Click the PNA application on the Windows taskbar
- Or press  on the front panel.

Copy Channels

You can copy the channel settings from an existing channel to a new or another existing channel.

[Why Copy Channels](#)

[How to Copy Channels](#)

[List of Channel Settings](#)

Other Setup Measurements Topics

Why Copy Channels

Copy channel settings if you need to create several channels that have slightly different settings.


For example, you have an amplifier that you want to characterize over a frequency span with several different input power levels.

Follow these steps:


1. Create one measurement with your optimized channel settings.
2. Copy that channel to new channels.
3. Change the power level on the new channels.

The alternative to using Copy Channels is to create new default measurements on new channels. Then change every channel setting to your new requirement. This is very time consuming and thus shows the benefit of the Copy Channels feature.

How to copy channels

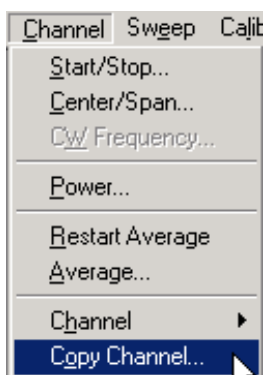

Learn more about using the [front panel interface](#)

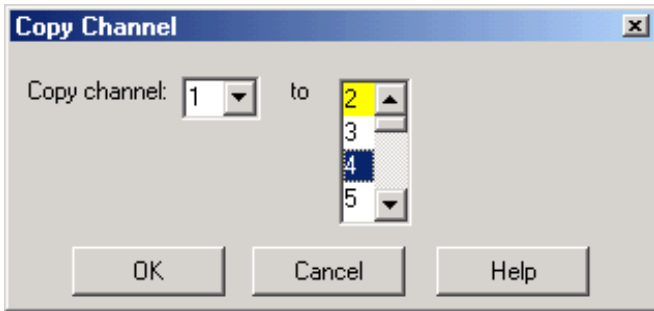

Copy Channel dialog box help

Copies an existing channel's settings to another channel.

Copy channel: Select a channel to copy.

to: Scroll to select a channel to copy settings to. Channel numbers that are currently being used are highlighted. They can be selected and overwritten.

Notes:

- You can copy channel settings to ONLY one new or existing channel. Repeat this operation to copy to more than one channel.
- The new channel is ALWAYS copied to the Active window. If you want the new channel in its own window, first create a new measurement in a new window. Then make sure it is the Active window before you copy the channel into it.
- The measurement in the new channel becomes the active measurement.
- Only the channel settings are copied. The measurement trace is NOT copied to the new channel.
 - If measurements already exist on a channel being copied to, the measurements on that channel will not change, but they will assume the new channel settings.
 - If a NEW channel is copied TO, an S11 measurement is created in order to view the channel settings.

For example:

1. **Existing** channel 1: S21 measurement
2. **Copy** channel 1 to NEW channel 2
3. **Result:** channel 2: S11 measurement with channel 1 copied settings. Both measurements are in the same window. The S11 measurement is the active measurement.

For more information see [Traces, Channels, and Windows on the PNA](#)

List of Channel Settings


- [Frequency Span](#)
- [Power](#)

- Cal Set usage
- Source Power Cal data
- IF Bandwidth
- Number of Points
- Sweep Settings
- Average
- Trigger (some settings)

Dynamic Range

Dynamic range is the difference between the analyzer receiver's maximum input power and the minimum measurable power (noise floor). For a measurement to be valid, input signals must be within these boundaries.

Increasing dynamic range is important if you need to measure very large variations in signal amplitude, such as filter bandpass and rejection. The dynamic range is shown below for an example measurement.

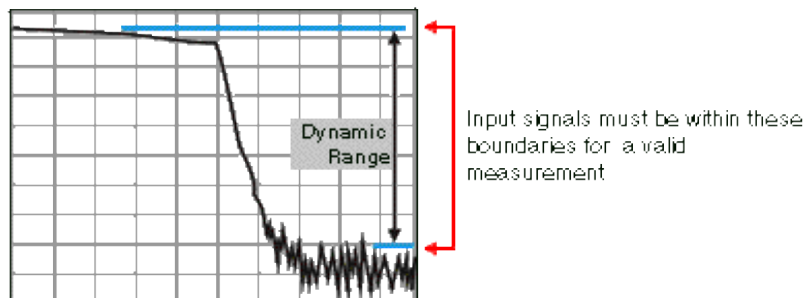

To help reduce measurement uncertainty, the analyzer dynamic range should be greater than the response that the DUT exhibits. For example, measurement accuracy is increased when the DUT response is at least 10 dB above the noise floor. The following methods can help you increase the dynamic range.

Increase the Device Input Power

Reduce the Receiver Noise Floor

Use the Front-Panel Jumpers (if your PNA has a configurable test set)

Other topics about Optimizing Measurements

Increase Device Input Power

Increase the DUT input power so that the analyzer can more accurately detect and measure the DUT output power. However, use caution - too much power can damage the analyzer receiver or cause compression distortion.

Caution! Receiver input damage level: +15 dBm.

increase input power to the device:

1. In the **Channel** menu, click **Power**
2. Select the **Power On** check box.
3. Under **Port Selection**, select the port that you are using as the source output.
4. In the **Test Port Power** box, type the value or press the arrow button to select the value you want.
5. Click **OK**.

Tip: You can further increase dynamic range by using an external booster amplifier to increase the input power to the DUT. See [High Power Amplifier Measurements](#).

Reduce the Receiver Noise Floor

You can use the following techniques to lower the noise floor and increase the analyzer's dynamic range.

- Reduce **crosstalk** between the PNA receivers when measuring signals close to the noise floor. See [Receiver Crosstalk](#).)
- Use **Sweep Averaging** - learn more about [Sweep Average](#)
- Reduce the **IF Bandwidth** - learn more about [IF Bandwidth](#).
- In [Segment sweep](#) mode each segment can have its own IF bandwidth. For example, when measuring a filter:
 - In the passband, the IF bandwidth can be set wider for a fast sweep rate, as long as high-level trace noise is kept sufficiently small.
 - In the reject band, where noise floor contributes significantly to measurement error, the IF bandwidth can be set low enough to achieve the desired reduction in average noise level.

Use the Front-Panel Jumpers (if your PNA has the configurable test set)

If your PNA has FOUR front-panel jumpers, you can bypass the test-port couplers and apply signals directly into the receivers. See [Dynamic Range - 4 Jumpers](#). Using this configuration, you can achieve up to 143 dB dynamic range with **Response Calibration** using segment sweep mode.

If your PNA has MORE THAN FOUR front-panel jumpers ([Configurable Test Set](#)), you can use the front-panel jumpers to reverse a test-port coupler. See [Dynamic Range - Configurable Test Set Option](#). Using this configuration, you can achieve up to 143 dB dynamic range with **Full 2-port Calibration** using segment sweep mode.

Note: Bypassing a port's directional coupler increases the port mismatch by approximately 15 dB (the coupling factor of the directional coupler).


- For information about upgrading your PNA to include front-panel jumpers, see [PNA Options](#).
- Discover the measurement possibilities using [front-panel jumpers](#).

Improving Dynamic Range with Configurable Test Set Option

To improve dynamic range you can reverse the signal path in the test-port coupler and bypass the loss typically associated with the coupled arm. As shown in the following graphic, the signal is applied to Port 2. The signal bypasses the coupled arm via the jumper cable connected to the Coupler Thru (or Coupler In) and the Receiver B In (or B In) ports. Using this configuration, you can increase the forward measurement dynamic range up to 143 dB with full 2-port calibration using segment sweep mode. When making full 2-port error corrected measurements, the reverse measurement is degraded by 15 dB, with up to 113 dB of dynamic range available.

Explore the graphic with your mouse.

Note: Your analyzer's block diagram may contain different components than shown below.

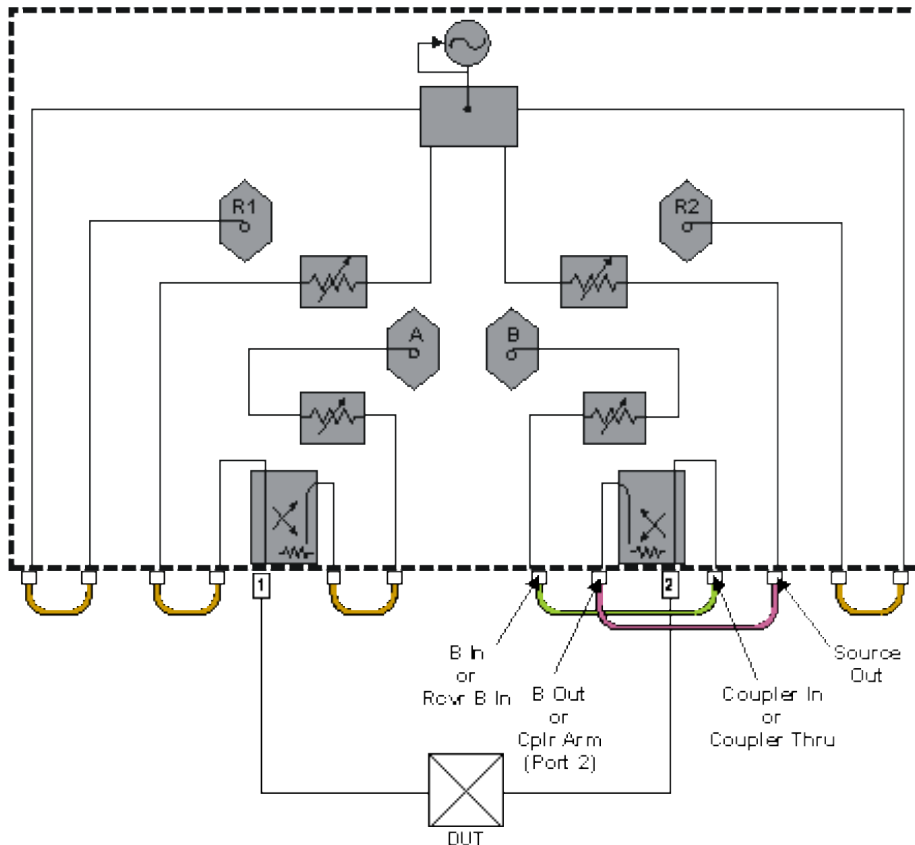

Number of Points

A data point or "point" is a sample of data representing a measurement at a single stimulus value. You can specify the number of points that the analyzer measures across a sweep. (A "sweep" is a series of consecutive data point measurements, taken over a sequence of stimulus values.)

The PNA sweep time changes proportionally with the number of points. However, the overall measurement cycle time does not. See [Technical Specifications](#) for more information on how the number of points, and other settings, affect the sweep time.

Note: You may experience a significant decrease in computer processing speed with increased number of points, number of traces, and calibration error terms (full 2-port or 3-port). If this becomes a problem, you can increase the amount of RAM with PNA [Option 022](#).

The default value is 201 points per sweep.

Other topics about Optimizing Measurements


Tips:

- To achieve the greatest trace resolution, use the maximum number of data points.
- For faster throughput use the smallest number of data points that will give you acceptable accuracy.
- To find an optimized number of points, look for a value where there is not a significant difference in the measurement when you increase the number of points.
- To ensure an accurate measurement [calibration](#), perform the calibration with the same number of points that will be used for the measurement.

How to change the number of data points


Use one of the following methods:

Select a number or click Custom to invoke a [dialog box](#)

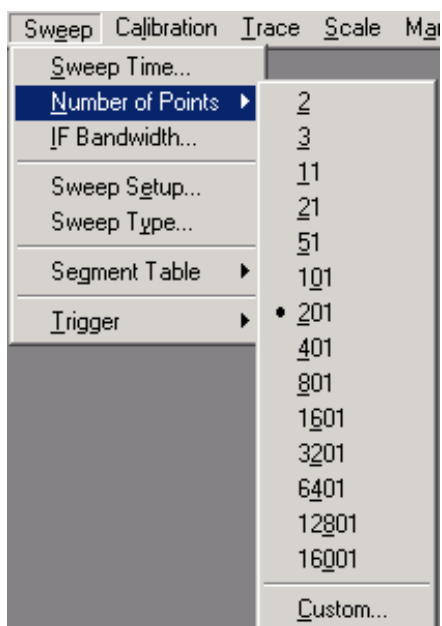



Learn more about using the [front panel interface](#)

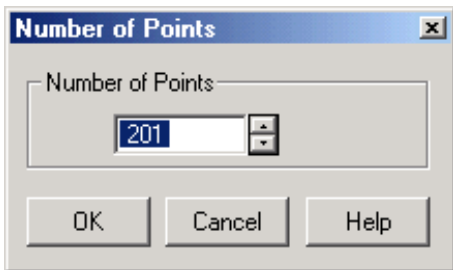

Number of Points dialog box help

Specifies the number of data points that the analyzer gathers during a measurement sweep.
You can specify any number from 2 to 16001.
The default value is 201.

Phase Measurement Accuracy

You can increase the accuracy of phase measurements by using the following PNA features.

[Electrical Delay](#)

[Port Extensions](#)

[Phase Offset](#)

[Spacing Between Frequency Points \(Aliasing\)](#)

[Learn more about Phase measurements](#)


Electrical Delay

Electrical delay is a mathematical function that simulates a variable length of lossless transmission line.


Use the electrical delay feature to compensate for the linear phase shift through a device. This feature allows you to look at only the deviation from linear phase of the device.

You can set the electrical delay independently for each measurement trace.

How to set Electrical Delay



Learn more about using the [front panel interface](#)

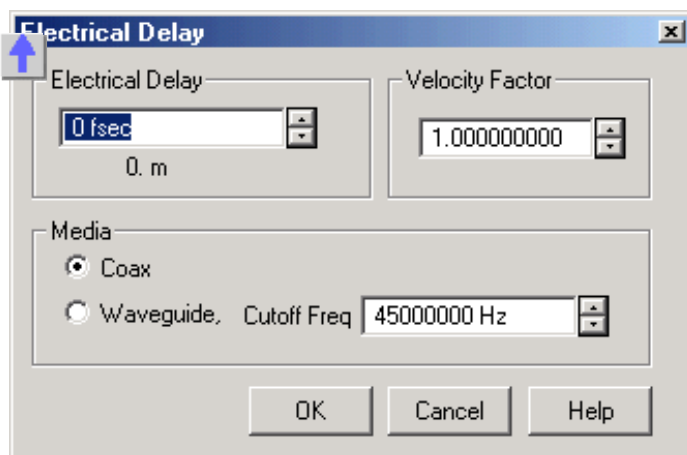

Electrical Delay dialog box help

Electrical Delay Specifies the value of delay added or removed, in units of time. This compensates for the linear phase shift through a device. You can set the electrical delay independently for each measurement trace.

Velocity Factor Specifies the relative velocity of the medium of the device inserted. The value for a polyethylene dielectric cable is 0.66 and 0.7 for Teflon dielectric.

Media

Coax select if the added length is coax. Also specify the velocity factor of the coax.

Waveguide Select if the added length is waveguide. Also specify the low frequency cutoff of the waveguide.

Cutoff Freq Low frequency cutoff of the waveguide.

Learn about [Electrical Delay](#) (scroll up)


Port Extensions

Use port extensions to electrically move the measurement reference plane after you have performed a calibration. The following two scenarios show how port extensions can be useful.

1. You have already performed a calibration, and then decide that you need to add a length of transmission line in the measurement configuration. Use port extensions to "tell" the analyzer you have added the length to a specific port.
2. You are unable to perform a calibration directly at your device because it is in a test fixture. Use port extensions to compensate for the time delay (phase shift), and optionally the loss, caused by the added transmission line of the fixture. See other [Fixture Compensation features](#).

Port extensions settings affect **all measurements on the active channel** that are associated with a particular port.

How to set Port Extensions

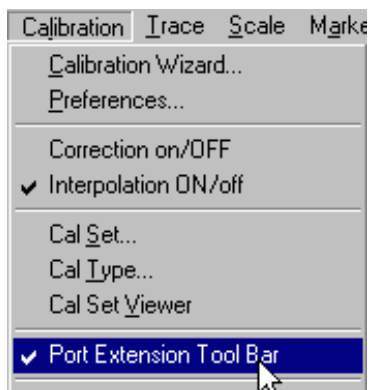

- To set port extensions, you need to know the length of additional transmission line, or you must be able to connect an OPEN or SHORT calibration standard at the point of the DUT. In most cases, removing the DUT will leave a suitable OPEN at the new reference plane.
- You can add port extension values manually or automatically. Both are performed with a calibrated measurement on the PNA.

Learn more about using the [front panel interface](#)



Port Extensions toolbar help

Learn about [Port Extensions](#) (scroll up)

- If you know the electrical length of additional transmission line, enter the value directly to the Delay setting.
- If you know the physical length of additional transmission line, increase the Delay setting until the physical length setting (directly above Delay) is achieved.
- If you do not know the electrical or physical length of additional transmission line, you must be able to connect an OPEN or SHORT to the new reference plane at the point of the DUT. In most cases, removing the DUT will leave a suitable OPEN at the new reference plane. Port Extensions can then be added manually (as follows), or by using [Automatic Port Extensions](#).

Manual Port Extensions Procedure

1. Select a calibrated S11 measurement.
2. Select Phase format.
3. With an OPEN or SHORT at the calibration reference plane, verify that the phase across the frequency span is at or near zero.
4. Connect the added transmission line or fixture and attach an OPEN or SHORT in place of the DUT. In most cases, removing the DUT will leave a suitable OPEN at the new reference plane. On the Port Extension toolbar, increase **Delay** until the phase response is flat across the frequency span of interest.
5. If you know the loss of the additional transmission line, enter the [Loss Compensation](#) values using either one or two data points.

Note: Most OPEN and SHORT standards have delay. Therefore, adjusting delay with this method results in a delay equal to two times the delay of the OPEN or SHORT.

Port Extensions Settings

Port Extension Turns ON and OFF port extensions on all ports.

Port Select a PNA port for delay and loss values. Port Extensions settings affect ALL measurements on the active channel that are associated with a particular port.

Delay The amount of port extension delay in time. To compensate for delay in additional transmission line, enter a positive value.

Loss Compensation

The following settings, along with [Loss at DC](#), allows the entire frequency span to be corrected for loss using a curved-fit algorithm.

To compensate for loss in additional transmission line, enter a positive value which causes the trace to shift in the positive (up) direction.

Loss1 Loss in dB at **Freq1**.

Use1 Check calculate and apply port extension Loss1 @Freq1 values. Also, check if using [Loss at DC value](#).

Loss2 Loss in dB at **Freq2**.

Use2 ONLY available if Use1 is checked. Calculate and apply port extension Loss2 @Freq2 values.

Loss is calculated for each frequency data point (f) as follows.

If Use1 is checked and NOT Use2 then:

$$\text{Loss}(f) = \text{Loss1} * (f/\text{Freq1}) ^ 0.5$$

If Use1 AND Use2 are checked, then:

$$\text{Loss}(f) = \text{Loss1} * (f/\text{Freq1}) ^ n$$

Where:

$$n = \log_{10} [\text{abs}(\text{Loss1}/\text{Loss2})] / \log_{10} (\text{Freq1}/\text{Freq2})$$


Note: abs = absolute value

More Invokes the More Port Extensions Settings dialog box.

Auto Ext. Invokes the Automatic Port Extensions dialog box

Note: Individual receiver port extensions (A,B, and so forth) can no longer be set. (Sept. 2004)

Learn about Port Extensions (scroll up)

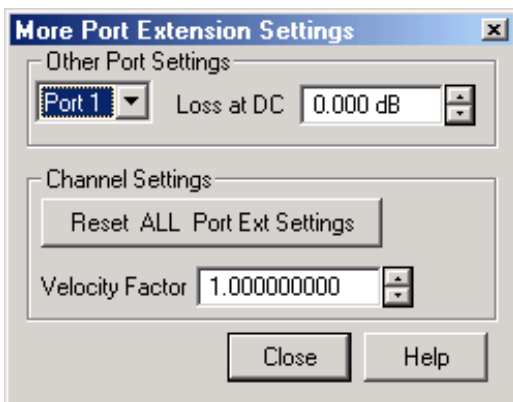

More Port Extensions Settings dialog box help

Note: Port Extensions settings affect ALL measurements on the **active** channel that are associated with a particular port.

Other Port Settings


Port - Loss at DC Offsets the entire frequency span by this value. Use1 on the Port Extension toolbar must also be checked. To compensate for loss at DC, enter a positive value which causes the trace to shift in the positive (up) direction.

Channel Setting

Reset ALL Port Ext Settings All port extensions settings are changed to preset values. Port Extension state (ON / OFF) is unaffected.

Velocity Factor Specifies the velocity factor that applies to the medium of the device that was inserted after the measurement calibration. The value for a polyethylene dielectric cable is 0.66 and 0.7 for Teflon dielectric. 1.0 corresponds to the speed of light in a vacuum.

Learn about Port Extensions (scroll up)

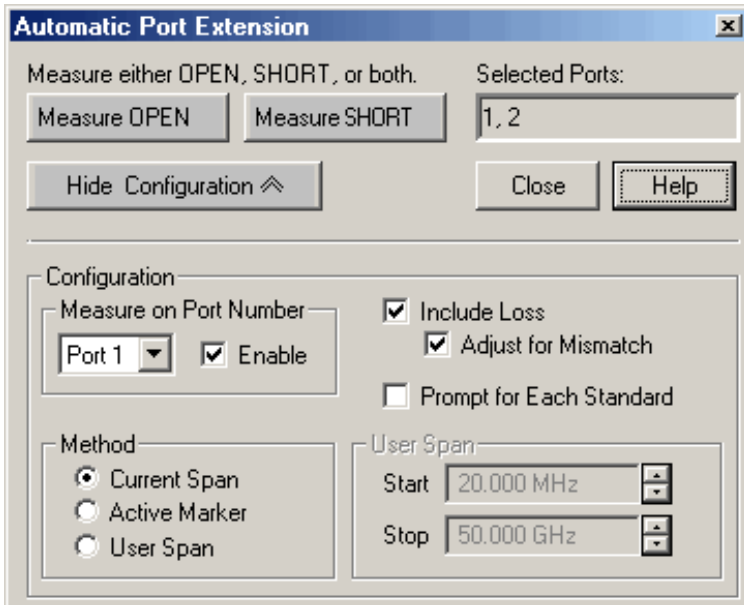

Automatic Port Extension dialog box help

Automatic Port Extension AUTOMATICALLY performs the same operation as [Manual Port Extension](#). By connecting a SHORT or OPEN, the reference plane is automatically moved to the point at which the standard is connected. In addition, Automatic Port Extension will optionally measure and compensate for the loss of the additional transmission line.

Auto Port Extensions Procedure

1. Connect the added transmission line or fixture. Attach an OPEN or SHORT to all affected ports at the new reference plane. In most cases, removing the DUT will leave a suitable OPEN at the new reference plane.
2. On the Port Extension toolbar, click **Auto Port Ext.** Click **Show Configuration** to make additional settings.
3. Click **Measure** to perform the port extension calculations. The resulting delay and loss settings are entered into the port extension toolbar. These settings are saved with Instrument Save or you can manually record the values and enter them again when required.

Settings

Measure either OPEN, SHORT, or both Press a button to make the measurement of the reflection standard.

Measure either OPEN or SHORT depending on which is most convenient. An ideal OPEN and SHORT, with zero loss and delay, is assumed. Therefore, accuracy is most affected by the quality of the standard. In most cases, removing the DUT will leave a suitable OPEN at the new reference plane. When measuring both OPEN and SHORT standards, the average of the two is used and will slightly improve accuracy.

Selected Ports Indicates the ports that currently have automatic port extension enabled. By default, ALL PNA ports are enabled. To disable a port, see **Measure on Port Number** below.

Note: Port Extensions settings affect ALL measurements on the active channel that are associated with a particular port.

Show/Hide Configuration Press to either show or hide the following configuration settings in the dialog box.

Measure on Port Number

Select port number to enable or disable automatic port extension.

Enable Check to enable the specified port. All enabled ports will have their reference plane automatically adjusted after performing Automatic Port Extension.

Include Loss Check to automatically measure the loss in the additional transmission line and apply compensation. To calculate loss compensation, frequencies at 1/4 and 3/4 through the frequency range are usually used as Freq1 and Freq2 values. [Learn more about Loss Compensation.](#)

Adjust for Mismatch Only available when **Include Loss** is checked. During the measurement of the OPEN or SHORT standard, mismatch could cause ripple in the magnitude (loss) response. The [Loss compensation curved-fit algorithm](#) allows half of the ripple to be positive and half negative. When measuring low-loss devices, it is possible that some magnitude responses could become slightly positive, indicating gain rather than loss.

Check - Offsets the trace to cause all of the data points to be at or below zero.

Clear - Most accurate application of the curve-fit calculation, but allows positive responses.

Prompt for Each Standard Check to invoke a prompt when the Measure OPEN or SHORT button is pressed. The prompt will indicate which standard to connect to which port.

Method

Select the span of data points which will be used to determine correction values for phase and loss (optional). If a portion of the current frequency span does not have flat or linear response, you can eliminate this portion from the calculations by using a reduced User Span.

To calculate loss compensation, Current Span and User Span methods usually use frequencies at 1/4 and 3/4 through the frequency range as Freq1 and Freq2 values. See [Loss Compensation](#) to learn more about how loss is calculated.

Current Span Use the entire frequency span to determine phase and loss values.

Active Marker Use only the frequency at the active marker, and one data point higher in frequency, to calculate phase and loss values. If a marker is not present, one will be created in the center of the frequency span.

User Span Use the following User Span settings to determine phase and loss values.

User Span

Start Enter start frequency of the user span.

Stop Enter stop frequency of the user span.


Learn about [Port Extensions](#) (scroll up)

Phase Offset


[Phase](#) offset mathematically adjusts the phase measurement by a specified amount, up to 360°. Use this feature in the following ways:

- **Improve the display of a phase measurement.** This is similar to the way you would change the reference level in an amplitude measurement. Change the phase response to center or align the response on the screen.
- **Emulate a projected phase shift in your measurement.** For example, if you know that you need to add a cable and that the length of that cable will add a certain phase shift to your measurement, you can use phase offset to add that amount and simulate the complete device measurement.

How to set Phase Offset



Learn more about using the [front panel interface](#)

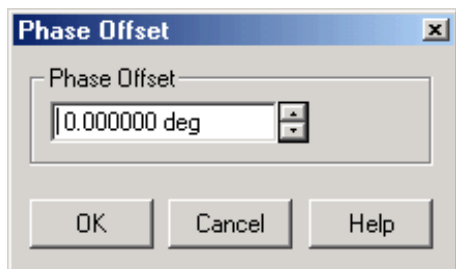

Phase Offset dialog box help

Phase Offset Type a value or use the up and down arrows to select any value up to 360 degrees.

Learn about [Phase Offset](#) (scroll up)


Spacing Between Frequency Points (Aliasing)

The analyzer samples data at discrete frequency points, then connects the points, creating a trace on the screen.

If the phase shift through a device is $>180^\circ$ between adjacent frequency points, the display can look like the phase slope is reversed. This is because the data is undersampled and aliasing is occurring.

If you are measuring group delay and the slope of the phase is reversed, then the group delay will change sign. For example, the following graphic shows a measurement of a SAW bandpass filter.

- The left measurement has 51 points and indicates the group delay is negative, which is a physical impossibility. That is, the response is below 0 seconds reference line.
- The right measurement shows an increase to 201 points which indicates the group delay is positive. That is, the response is above the 0 seconds reference line.

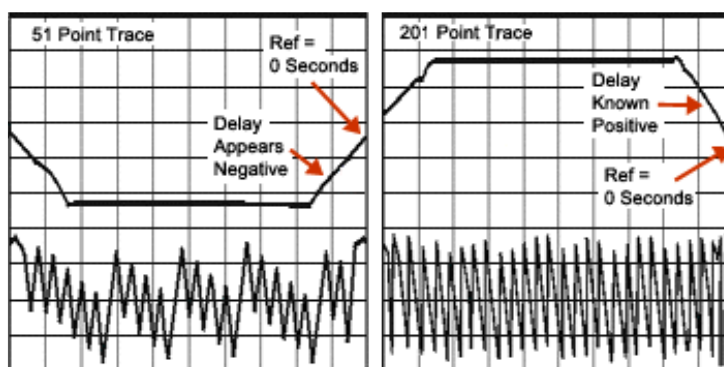

Tip: To check if aliasing might be occurring in a measurement, either increase the number of points or reduce the frequency span.

Electrically-Long Device Measurements

A signal coming out of a device under test may not be exactly the same frequency as the signal going in to a device at a given instant in time. This can sometimes lead to inaccurate measurement results. You can choose between two techniques to eliminate this situation and increase measurement accuracy.

Why Device Delay May Create Inaccurate Results

Solutions to Increase Measurement Accuracy

Slow the Sweep Speed


Add Electrical Length to the R Channel

Other topics about Optimizing Measurements

Why Device Delay May Create Inaccurate Results

The following graphic shows an example of this situation:

- In the network analyzer, the source and receiver are phase locked together and sweep simultaneously through a span of frequencies.
- The signal flow through the Device Under Test (DUT) is shown as different colors for different frequencies.
- You can see as a stimulus frequency travels through the DUT, the analyzer tunes to a new frequency **just before** the signal arrives at the receiver. This causes inaccurate measurement results.

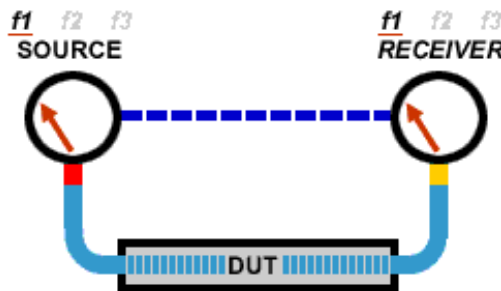

If the analyzer is measuring a long cable, the signal frequency at the end of the cable will lag behind the network analyzer source frequency. If the frequency shift is appreciable compared to the network analyzer's IF detection bandwidth (typically a few kHz), then the measured result will be in error by the rolloff of the IF filter.

Note: There is no fixed electrical length of a device where this becomes an issue. This is because there are many variables that lead to measurement speed. When high measurement accuracy is critical, lower the sweep speed until measurement results no longer change.

Solutions to Increase Measurement Accuracy

Choose from the following methods to compensate for the time delay of an electrically long device.

Slow the Sweep Speed

Add Electrical Length to the R Channel

Slow the Sweep Speed

The following methods will slow the sweep speed.

Increase the Sweep Time

Increase the Number of Points

Use Stepped Sweep

Set Dwell Time


Add Electrical Length to the R Channel

Note: This method applies to PNA models with front panel loops.

Instead of slowing the sweep, you can compensate for the electrical length of a cable or fixture.

- a. Remove the R-channel jumper on the front panel of the analyzer.
- b. Replace the jumper with a cable of about the same length as the device under test.
 1. Add the cable on the R1 channel for S₁₁ and S₂₁ measurements.
 2. Add the cable on the R2 channels for S₂₂ and S₁₂ measurements.
- c. Set the analyzer for a fast sweep.

Configuration for S₂₂ and S₁₂ Measurements

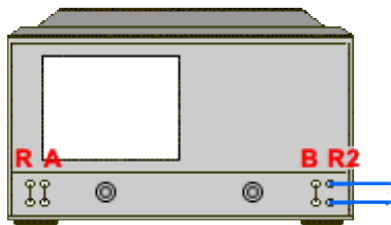

This method balances the delays in the reference and test paths, so that the network analyzer's ratioed transmission measurement does not have a frequency-shift error.

Note: This method works well if the delay is in a cable or fixture. For devices with long delays, this method is only suitable for uncalibrated measurements.

Reflection Accuracy on Low-Loss 2-Port Devices

To make accurate reflection measurements that have a 1-port calibration, you should terminate the unmeasured port.

[Why Terminate the Unmeasured Port](#)

[How to Terminate the Unmeasured Port](#)

[Resulting Measurement Uncertainty](#)

Other topics about Optimizing Measurements


Why Terminate the Unmeasured Port

A 2-port calibration corrects for all 12 twelve error terms. A 1-port calibration corrects for directivity, source match and frequency response, but not load match. Therefore, for highest accuracy, you must make the load match error as small as possible. This especially applies for low-loss, bi-directional devices such as filter passbands and cables. You do not need to be concerned with load match when you are measuring a device with high reverse isolation, such as an amplifier.

How to Terminate the Unmeasured Port

Use one of the following methods:

- Connect a high-quality termination load (from a calibration kit, for example) to the unmeasured port of your device. This technique yields measurement accuracy close to that of a Full SOLT 2-port calibration.
- Connect the unmeasured port of your device directly to the analyzer, inserting a 10 dB precision attenuator between the device output and the analyzer. This improves the effective load match of the analyzer by approximately twice the value of the attenuator, or 20 dB.

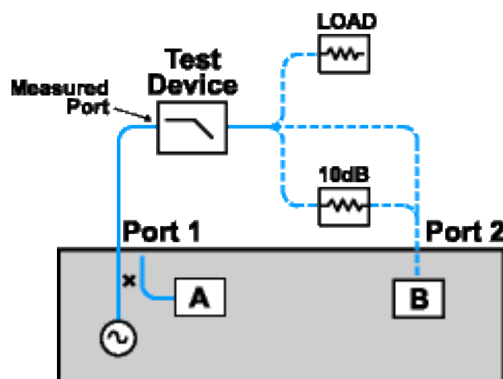

Resulting Measurement Uncertainty

The following graph illustrates the measurement uncertainty that results from terminating **with** and **without** a precision 10 dB attenuator on the output of the test device.



Legend

- Filter Reflection
- Uncertainty **with** attenuator
- Uncertainty **without** attenuator

The calculations below show how adding a high-quality 10 dB attenuator improves the load match of the analyzer.

Note: The corresponding linear value is shown in parentheses.

Network Analyzer:

Load match (NA_{LM}) = 18 dB (.126)

Directivity (NA_D) = 40 db (.010)

Filter:

Insertion loss (F_{IL}) = 1dB (.891)

Return loss (F_{RL}) = 16 dB (.158)

Attenuator:

Insertion loss (A_{IL}) = 10 dB (.316)

SWR (A_{SWR}) = 1.05 (.024)

32.26 dB Return Loss

Calculations:

Without Attenuator

$$\begin{aligned} r_{NA} &= (FIL) * (NALM) * (FIL) \\ &= (.891) * (.126) * (.891) \\ &= .100 \end{aligned}$$

$$r_{Attenuator} = NA$$

$$\begin{aligned} \text{Worst Case Error (EWC)} &= \rho_{NA} \\ &= .1 \end{aligned}$$

With Attenuator

$$\begin{aligned} &= (FIL) * (AIL) * (NALM) * (AIL) * (FIL) \\ &= (.891) * (.316) * (.126) * (.316) * (.891) \\ &= .010 \end{aligned}$$

$$\begin{aligned} &= (FIL) * (ASWR) * (FIL) \\ &= (.891) * (.126) * (.891) \\ &= .019 \end{aligned}$$

$$\begin{aligned} &= \rho_{NA} + \rho_{Attn.} \\ &= .01 + .019 \\ &= .029 \end{aligned}$$

$$\begin{aligned} \text{Uncertainty Adds} &= -20\log(FRL) + (EWC) + (NAD) \\ &= -20\log(.158) + (.100) + (.010) \\ &= \mathbf{11.4 \text{ dB}} \end{aligned}$$

$$\begin{aligned} &= -20\log(FRL) + (EWC) + (NAD) \\ &= -20\log(.158) + (.029) + (.010) \\ &= \mathbf{14.1 \text{ dB}} \end{aligned}$$

$$\begin{aligned} \text{Uncertainty Subtracts} &= -20\log(FRL) - (EWC) - (NAD) \\ &= -20\log(.158) - (.100) - (.010) \\ &= \mathbf{26.4 \text{ dB}} \end{aligned}$$

$$\begin{aligned} &= -20\log(FRL) - (EWC) - (NAD) \\ &= -20\log(.158) - (.029) - (.010) \\ &= \mathbf{18.5 \text{ dB}} \end{aligned}$$

Measurement Stability

There are several situations that can cause unstable measurements. To ensure that you are making repeatable measurements, you can use various methods to create a stable measurement environment.

[Frequency Drift](#)

[Temperature Drift](#)

[Inaccurate Measurement Calibrations](#)

[Device Connections](#)

Other topics about Optimizing Measurements

Frequency Drift

The analyzer frequency accuracy is based on an internal 10 MHz frequency oscillator. See [Technical Specifications](#) for stability and aging specifications.

If your measurement application requires better frequency accuracy and stability, you can override the internal frequency standard and provide your own high-stability external frequency source through the [10 MHz Reference Input connector on the rear panel](#).

Temperature Drift

Thermal expansion and contraction changes the electrical characteristics of the following components:

- Devices within the analyzer
- Calibration kit standards
- Test devices
- Cables
- Adapters



To reduce the effects of temperature drift on your measurements, do the following.

- Switch on the analyzer 1/2 hour before performing a measurement calibration or making a device measurement.
- One hour before you perform a measurement calibration, open the case of the calibration kit and take the standards out of the protective foam.
- Use a temperature-controlled environment. All specifications and characteristics apply over a 25 °C \pm 5 °C range (unless otherwise stated).
- Ensure the temperature stability of the calibration kit devices.
- Avoid handling the calibration kit devices unnecessarily during the calibration procedure.
- Ensure the ambient temperature is \pm 1°C of the measurement calibration temperature.

Inaccurate Measurement Calibrations

If a measurement calibration is inaccurate, you will not measure the true response of a device under test. To ensure that your calibration is accurate, you should consider the following practices:

- Perform a measurement calibration at the points where you connect the device under test, that is, the reference plane.
- If you insert any additional accessory (cable, adapter, attenuator) to the test setup after you have performed a measurement calibration, use the port extensions function to compensate for the added electrical length and delay.
- Use calibration standards that match the definitions used in the calibration process.
- Inspect, clean, and gage connectors. See Connector Care.

See Accurate Measurement Calibrations for more detailed information.

Device Connections

Good connections are necessary for repeatable measurements. To help make good connections, do the following:

- Inspect and clean the connectors for all of the components in the measurement setup.
- Use proper connection techniques.
- Avoid moving the cables during a measurement.

Noise Reduction Techniques

Random electrical noise which shows up in the analyzer receiver chain can reduce measurement accuracy. The following PNA functions help reduce trace noise and the noise floor which can lead to better dynamic range and more accurate measurements.

Note: The trace noise in microwave PNAs becomes worse below 748 MHz and is especially obvious between 10 MHz and 45 MHz. See Reduce IFBW.

Sweep Average

IF Bandwidth

Trace Smoothing

See Increase Dynamic Range to learn more about improving this critical parameter.


Other topics about Optimizing Measurements

Sweep Average

Sweep average is a feature that reduces the effects of random noise on a measurement. The PNA computes each data point based on the average of the same data point over several consecutive sweeps. You determine the number of consecutive sweeps by setting the Average factor. The higher the average factor, the greater the amount of noise reduction.



- When Averaging is ON, an **Average Counter** appears on the screen displaying the number of sweeps that has been averaged. The effect on the signal trace can be viewed as the Average Factor increases. This can assist in the selection of the optimum number of sweep averages.
- Averaging is applied to all measurements in a channel. The Average counter is displayed for each channel.
- Averaging for unratiod (single receiver) measurements is calculated differently from ratio measurements. for example, For an Averaging Factor of 2:
 - **Ratiod** measurements: $(re1 + re2) / 2 ; (imag1 + imag2) / 2$
 - **Unratiod** measurements: $(mag1 + mag2) / 2 ; (phase1 + phase2) / 2$. Magnitude results are valid, but phase results are not valid. This is because phase measurements are relative by nature. Measuring absolute phase with a single receiver appears random. Averaging random positive and negative numbers will tend toward 0. Also, The noise floor does not drop when averaging unratiod measurements as on ratiod measurements.
- Use Average and IF bandwidth for the same benefit of general noise reduction. For minimizing very low noise, using Average is more effective than reducing system bandwidth. Generally, Averaging takes slightly longer than IF Bandwidth reduction to lower noise, especially if many averages are required.

Effects of Sweep Average

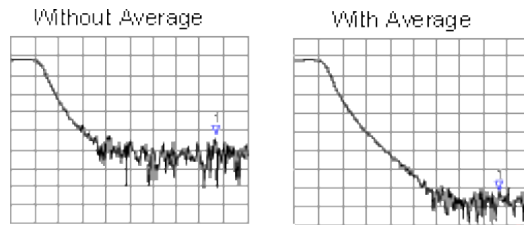


How to Set Averaging

Use one of the following methods:

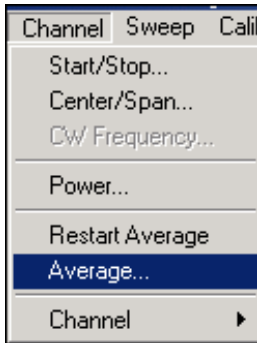

Learn more about using the [front panel interface](#)

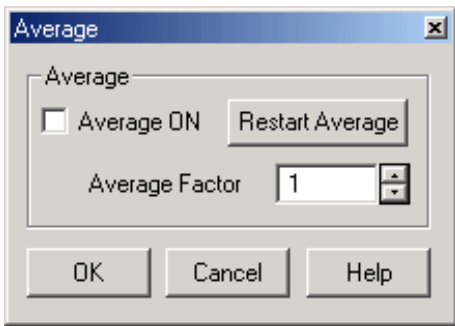

Average dialog box help

Average ON

Checked - Averaging is applied
 Cleared - Averaging is NOT applied

Average Factor Specifies the number of sweeps that is averaged. Range of 1 to 1024.

Restart Begins a new set of measurements that are used for the average. This set of measurements is equal to the average factor.

[Learn about Averaging](#) (scroll up)


IF Bandwidth

The PNA converts the received signal from its source to a lower intermediate frequency (IF). The bandwidth of the IF bandpass filter is adjustable from 40 kHz (for most PNA models) down to a minimum of 1 Hz.


Reducing the IF receiver bandwidth reduces the effect of random noise on a measurement. Each tenfold reduction in IF bandwidth lowers the noise floor by 10 dB. However, narrower IF bandwidths cause longer sweep times.

You can set the IF bandwidth independently for each channel or each segment of segment sweep.


Effect of Reducing IF Bandwidth

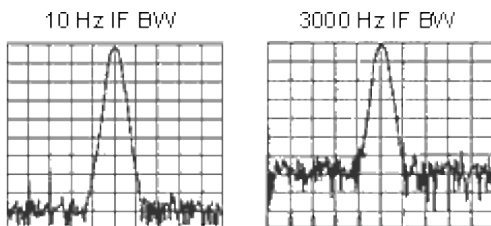

How to set IF Bandwidth



Learn more about using the [front panel interface](#)

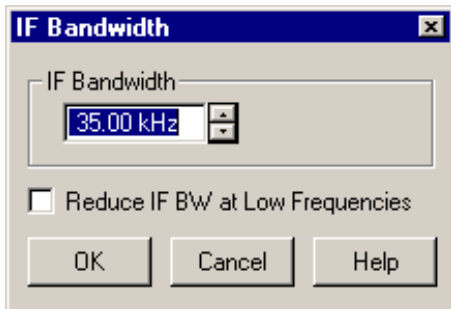

[IF Bandwidth dialog box help](#)

IF Bandwidth Specifies the IF (receiver) bandwidth. The value of IF bandwidth is selected by scrolling through the values available in the IF bandwidth text box. The IFBW is set independently for each channel.

The list of selectable IF Bandwidths vary with PNA model.

- The following values are common to all models: **1 | 2 | 3 | 5 | 7 | 10 | 15 | 20 | 30 | 50 | 70 | 100 | 150 | 200 | 300 | 500 | 700 | 1K | 1.5K | 2K | 3K | 5K | 7K | 10K | 15K | 20K | 30K**
- In addition, the following values are PNA Model specific:
 - N5230A Opt 220/225/420/425/520/525: **50K | 70K | 100K | 150K | 200K | 250K**
 - N5230A Opt 240/245: **50K | 70K | 100K | 150K | 200K | 280K | 360K**
 - All other PNAs: **35K | 40K**

OK Selects the value of IF bandwidth shown in the text box.

[Learn about IF Bandwidth](#) (scroll up)

Reduce IF BW at Low Frequencies

Note: This setting is **ONLY** available on 2-port PNA models with 20 GHz or higher maximum frequency.

The trace noise on these models becomes worse below 748 MHz. This is especially obvious between 10 MHz and 45 MHz and also when Time Domain is ON.

When this box is checked, the PNA uses a smaller IF Bandwidth at lower stimulus frequencies than the selected value, which reduces trace noise.

This setting is ON (checked) by default. Each channel can be set individually.

Use the following calculations to determine the actual IF Bandwidth value:

- For measurements from 10 MHz to 45 MHz:
Actual IF BW = (selected IF BW) x (.025)
- For measurements from 45 MHz to 748 MHz:
Actual IF BW = (selected IF BW) x (.5)

If the result is NOT a selectable IF BW value, the next higher selectable value is used.

Example:

Selected IF BW: 30 KHz

From **10 MHz to 45 MHz**: 30,000Hz * .025 = 750 Hz (PNA uses **1000 Hz**.)

From **45 MHz to 748 MHz**: 30,000Hz * .5 = **15 KHz**

From **748 MHz** to stop sweep: **30 KHz**

This setting also applies to [segment sweep](#).

Trace Smoothing

Trace smoothing averages a number of adjacent data points to smooth the displayed trace. The number of adjacent data points that get averaged together is also known as the smoothing aperture. You can specify aperture as either the number of data points or the percentage of the x-axis span.


Trace Smoothing reduces the peak-to-peak noise values on broadband measured data. It smooths trace noise and

does not increase measurement time significantly.


Tips:

- Start with a high number of display points and reduce until you are confident that the trace is not giving misleading results.
- Do not use smoothing for high-resonance devices, or devices with wide trace variations. It may introduce measurement errors.
- You can set the smoothing function independently for each trace.


Effects of Smoothing on a Trace

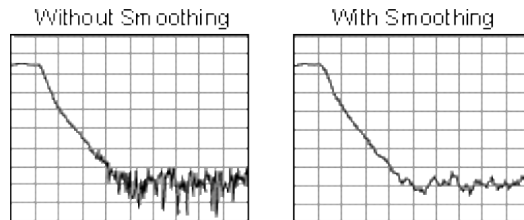

How to set Trace Smoothing

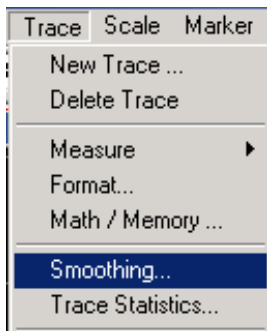

Learn more about using the [front panel interface](#)

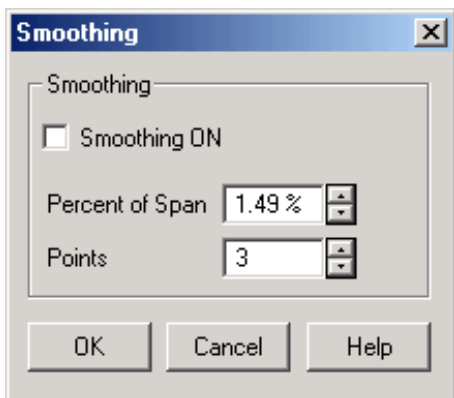

Smoothing dialog box help

Smoothing ON When checked, applies the smoothing function that averages data over a portion of the displayed trace.

Percent of Span Specifies the smoothing aperture as a percent of the swept stimulus span. For example, with a 401 points specified, the percent span is between 0.19% and 25%.

Points Specifies the smoothing aperture as a percent of the total number of measurement points in the swept stimulus span.

[Learn about Trace Smoothing](#) (scroll up)

Crosstalk

Crosstalk is energy leakage between analyzer signal paths. This can be a problem with high-loss transmission measurements. However, you can reduce the effects of crosstalk by doing the following:

[Set the Sweep to Alternate](#)

[Perform an Isolation Calibration](#)

Other topics about Optimizing Measurements

Set the Sweep to Alternate

Alternate sweep measures only one receiver per sweep. When one receiver is measured, the analyzer switches off the other receiver. This helps reduce receiver crosstalk.

Note: Alternate sweep mode can be set independently for each measurement channel. If multiple measurement channels are in use, you may want to set Alternate sweep for each channel.

1. In the **Sweep** menu, click **Sweep Setup**.
2. Check **Alternate Sweeps**.
3. Click **OK**.

Tips:

- The analyzer measures reflection (Receiver A) and transmission (Receiver B) on separate sweeps. Therefore, when the analyzer is making both reflection and transmission measurements, alternate sweep doubles the sweep cycle time.
- For transmission only or reflection only measurements, you can use alternate sweep to minimize the effects of crosstalk without affecting the sweep cycle time.
- The noise floor has to be lowered substantially before crosstalk is visible. You may need to use the average function or narrow the IF bandwidth.



Perform an Isolation Calibration

For transmission measurements, a response and isolation measurement calibration helps reduce crosstalk because the analyzer measures and then subtracts the leakage signal during the measurement calibration. The calibration improves isolation so that it is limited only by the noise floor.

See [Isolation error](#) to learn how crosstalk can be reduced in the calibration process.

Generally, the isolation error falls below the noise floor. So when you are performing an isolation calibration you should use a noise reduction technique such as sweep averages or reducing the IF bandwidth.

Effects of Accessories

Accessories in a configuration may affect the results of a device measurement. You can choose between two analyzer features that reduce the effects of accessories.

Power Slope to Compensate for Cable Loss

Gating to Selectively Remove Responses

Other topics about Optimizing Measurements

Power Slope to Compensate for Cable Loss

If you have a long cable or other accessory in a measurement configuration where a power loss occurs over frequency, apply the power slope function. This function increases the analyzer source power by a rate that you define (dB/GHz).

1. In the **Channel** menu, click **Power**.
2. If the slope function is not already switched on, click the **Slope** check box.
3. In the **dB/GHz** box, enter the rate that you want the source power to increase over the frequency sweep. Click **OK**.

Gating to Selectively Remove Responses

Gating is a feature in the time domain (option 010) that allows the analyzer to mathematically remove responses. You can set the gate for either a reflection or transmission response, but you will see different results.

- **Gating a reflection response** isolates a desired response (such as a filter's return loss), from unwanted responses (such as adapter reflections or connector mismatches).
- **Gating a transmission response** isolates a specific path in a multipath device that has long electrical lengths.



See [Time Domain Gating](#) for more information.

Fast Sweep Speed

Maintaining the fastest measurement sweep is one aspect of achieving the best measurement throughput. You can make the analyzer have the fastest sweep for your measurement application by adjusting the following:

Sweep Settings

Noise Reduction Settings

Measurement Calibration Choice

Unnecessary Functions

Other topics about Optimizing Measurements

Sweep Settings

Consider changing each of the following settings as suggested.

Frequency Span - Measure only the frequencies that are necessary for your device.

Segment Sweep - Use segments to focus test data only where you need it.

Switch Off Stepped Sweep - Use linear swept mode to minimize sweep time when possible.

Auto Sweep Time - Use this default to sweep as quickly as possible for the current settings.

Number of Points - Use the minimum number of points required for the measurement.

For more information on how number of points and other settings affect sweep cycle time, see [Technical Specifications](#).

Noise Reduction Settings

Using a combination of these settings, you can decrease the sweep time while still achieving an acceptable measurement.

IF Bandwidth. Use the widest IF bandwidth that will produce acceptable trace noise and [dynamic range](#).

 **verage**. Reduce the average factor, or switch Average off.

Measurement Calibration Choice

Choose the fastest type of [calibration](#) for the required level of accuracy.

- Sweep speed is about the same for uncorrected measurements and measurements done using a response calibration, or one-port calibration.
- A full two-port calibration requires both forward and reverse sweeps to update all four S-parameters for error correction, even when only a single S-parameter is displayed.

For more information see [Select a Calibration](#).

Unnecessary Functions

The analyzer must update information for all active functions. To achieve an additional increase in sweep speed,

switch off all of the analyzer functions that are not necessary for your measurement application.

Delete Unwanted Traces

1. Click on the Trace Status bar to make an unnecessary trace active.
2. In the **Trace** menu, click **Delete Trace**.

Switch Off Unwanted Markers

1. In the **Marker** menu, click **Select Marker**, and click an unwanted marker on the list.
 - If you want to switch off all of the markers, click **All Off**.
2. Display the Marker toolbar: from the **View** menu, click **Toolbars**, and then click **Marker**.
3. Clear the **On** checkbox to switch off the marker.

Switch Off Smoothing

1. In the **Trace** menu, click **Smoothing**.
2. Click the **Smoothing On** box to clear the checkbox, switching off the smoothing function. Click **OK**.

Switch Off Limit Testing

1. In the **Trace** menu, click **Limit Test**.
2. Click the **Limit Test ON** box to clear the checkbox, switching off the limit function. Click **OK**.

Switch Off Math Functions

- In the **Trace** menu, point to the **Data Math** list and click **Data** to view only the current measurement trace.

Analyzer sweep speed is dependent on various measurement settings. Experiment with the settings to get the fastest sweep and the measurement results that you need.

Switch Between Multiple Measurements

If you need to make multiple measurements to characterize a device, you can use various methods to increase throughput. Experiment with these methods to find what is best for your measurement application needs.

[Set Up Measurements for Increased Throughput](#)

[Arrange Measurements in Sets](#)

[Use Segment Sweep](#)

[Trigger Measurements Selectively](#)

[Automate Changes Between Measurements](#)

[Recall Measurements Quickly](#)

[Other topics about Optimizing Measurements](#)

Set Up Measurements for Increased Throughput

To achieve optimum throughput of devices that require multiple measurements, it is helpful to know the operation of the PNA. This knowledge allows you to set up the measurement scenarios that are best for your applications.


[Learn more about Traces, Channels, and Windows on the PNA](#)

Arrange Measurements in Sets

If you arrange measurements to keep the complete set of device measurements in one instrument state, you can save them so that you can later recall a number of measurements with one recall function.

See [Pre-configured Measurement Setups](#) for more information.

Use Segment Sweep

 Segment sweep is helpful if you need to change the following settings to characterize a device under test.

- Frequency Range
- Power Level
- IF [Bandwidth](#)
- Number of Points

The segment sweep allows you to define a set of frequency ranges that have independent attributes. This allows you to use one measurement sweep to measure a device that has varying characteristics.

See [Segment Sweep](#) for more information.

Trigger Measurements Selectively

You can use the measurement trigger to make measurements as follows:

- Continuously update only the measurements that have rapidly changing data.
- Occasionally update measurements that have infrequently changing data.

For example, if you had four channels set up as follows:

- Two channels measuring the data that is used to tune a filter
- Two channels measuring the data for the out-of-band responses of the filter

You would want to constantly monitor only the measurement data that you use for tuning the filter. If you continuously update all of the channels, this could slow the response of the analyzer so that you would not be able to tune the filter as effectively.

Note: You must either trigger the infrequent measurement manually or with remote interface commands.

To trigger measurements selectively:

This procedure shows you how to set up two different measurements with the following behavior:

- Channel 1 measurement will continuously update the data.
- Channel 2 measurement will occasionally update the data.

1. In the **Windows** menu, click **Meas Setups, Setup D**.

Set Up a Measurement Trigger for Continuous Updates

2. In the **Sweep** menu, click **Trigger, Trigger...**
3. Under **Trigger Source**, click **Internal**.
4. Under **Channel Trigger State**, select **Channel 1**, and click **Continuous**.

Set Up a Measurement Trigger for Occasional Updates

5. Under **Channel Trigger State**, select **Channel 2**, and click **Single, OK**.
 - If you want the analyzer to trigger more than a single sweep, click the **Enable Groups** check box and enter the number of sweeps.
6. In the **System** menu, click **Keys, Trigger**.

Update the Measurement

7. Click on the lower window to make Channel 2 the active channel.
8. On the active entry toolbar, click the type of trigger you set up.
 - Click **Single** if you set up the analyzer for a single sweep per trigger.
 - Click **Groups** if you set up the multiple sweeps per trigger.

Note: A trace must be active for you to initiate a trigger for that measurement.

Automate Changes Between Measurements

If there are slight differences between the various measurements that you need to characterize a device, you may find that it is faster to change the measurement settings using programming.

Recall Measurements Quickly

The most efficient way to recall measurements is to recall them as a set of measurements (instrument state).


- It only takes a short time longer to recall an instrument state that includes multiple measurements, than it does to recall an instrument state with only one measurement.
- Each recall function has time associated with it. You can eliminate that time by setting up the measurements as a set so you can recall them as a set.

See [Save and Recall Files](#) for more information.

Data Transfer Speed

The fastest data transfer helps you achieve the best measurement throughput. Try these methods for improving data transfer speed.

- **Use single sweep mode** to ensure that a measurement is complete before starting a data transfer.
1. In the **Sweep** menu, click **Trigger, Trigger...**
 2. Under **Trigger Source**, click **Manual**.
 3. Under **Channel Trigger State**, select the channel for the measurement that you want to transfer, and click **Continuous, OK**.
 4. Update the Measurement
 1. In the **System** menu, click **Keys, Trigger**
 2. In the active entry toolbar, click **Single**
- **Transfer the minimum amount of data** needed. For example, a trace with a few points, using segment sweep rather than a full trace with many linearly spaced points. Also, use markers instead of trace transfers.
 - **Choose the REAL data format** to provide the fastest transfer speed when using SCPI programs for automated applications.
 - **Use SCPI over LAN** for applications that are automated with SCPI programs.
 - **Use COM programs** to provide the fastest transfer speed when using an automated application. See [Data Transfer Time](#).

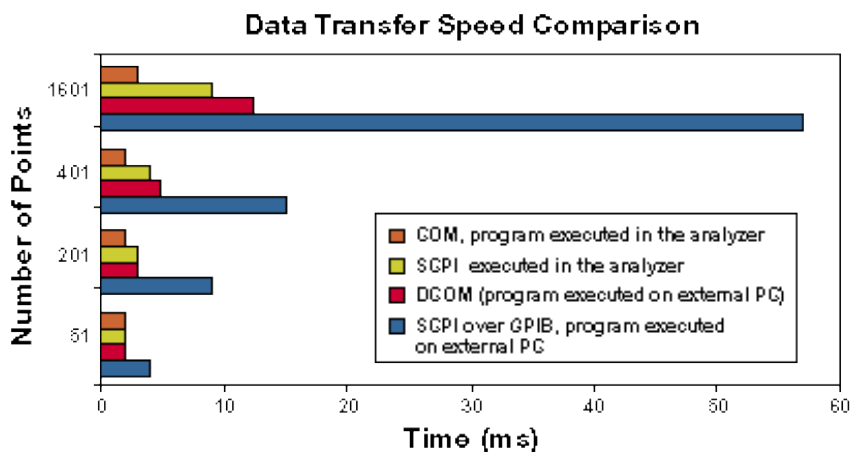

[Other topics about Optimizing Measurements](#)

Using Macros

Macros are executable programs that you write, load into the analyzer, and then run from the analyzer. You can have up to 12 macros set up to run on the analyzer.


[How to Setup Macros](#)

[How to Run Macros](#)

[Macro Example](#)

How to Setup Macros

Use one of the following methods to access the Macro Setup dialog box:

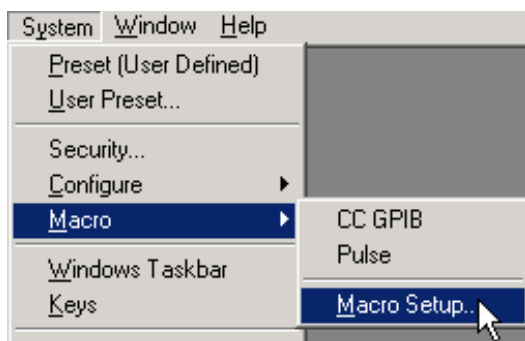

1.



2.

In the Macro Setup dialog box:

1. Click on a blank line below the last entry. (There may be NO entry.)

 Click **Edit**

3. In the **Macro Title** box, type a descriptive title for your macro.

4. Click **Browse**.


5. Change **Files of Type**

6. Find and click your macro file

7. Click **OK**

8. Click **OK** on the Macro Setup dialog box.

Learn more about using the [front panel interface](#)

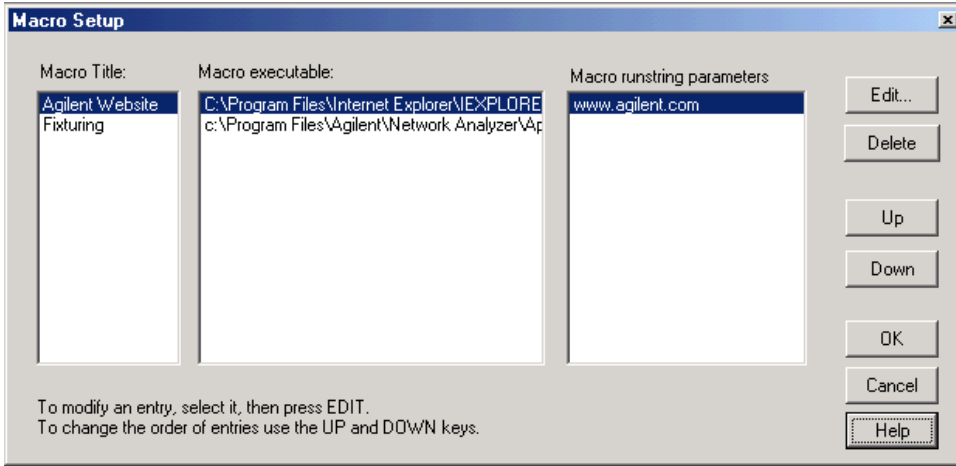

Macro Setup dialog box help

Allows you to create a set of 12 macros so that you can launch other programs from within the PNA application.

To add a Macro, select a blank line then click **Edit**

Macro Title Shows the titles that appear in the active entry toolbar when you press the Macro key. These titles are associated with the executable files and should be descriptive so you can easily identify them. For example, if you wanted to launch the Agilent Home Page, you could title the executable "Agilent Home."

Macro Executable Lists the complete path to the executable file. To follow the example of launching the Agilent PNA Series Home Page, the path to the executable could be "C:\Program Files\Internet Explorer\iexplore.exe."


Macro Runstring Parameters Lists the parameters that get passed to the program that is referenced in the executable file. Again following the example of launching the PNA Series Home Page, you could assign the runstring parameters "http://www.agilent.com/find/pna".

Edit Invokes the Macro Edit dialog box.

Delete Deletes the selected macro.

Up Allows you to reorder the macros, moving the selected macro up one line. For the 12 possible macros there are 12 lines, indicating the order that they appear in the active entry toolbar when you press the Macro key. Since there are four titles that can be shown at one time in the toolbar, when you repeatedly press the Macro key, the toolbar changes the macro titles to the next set of four macro titles.

Down Moves the selection down one line in the list of macros.

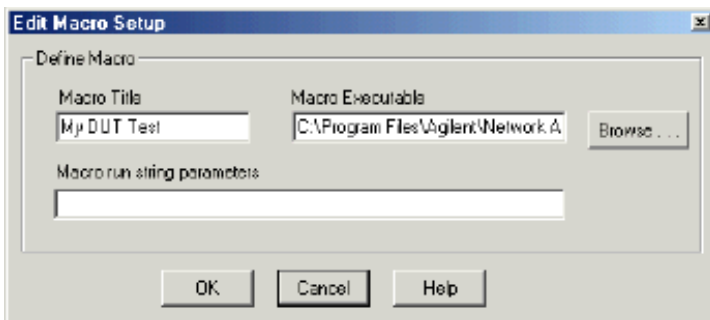

Macro Edit dialog box help

Macro Title Allows you to modify the title that appears in the active entry toolbar.

Macro Executable Allows you to modify the complete path to the macro executable file.

Browse Allows you to look through drives and directories, to locate the macro executable file and establish the complete path to the file.


Macro run string parameters Allows you to modify the parameters that are passed to the program referenced in the executable file.

[See Macro Setup dialog box](#)

How to Run Macros

Use one of the following methods to run a Macro:

1.  Press until your macro is visible, then 

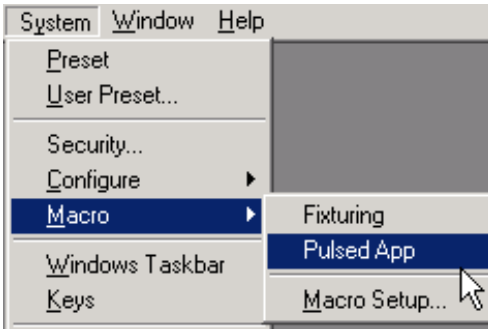2. 
Select your Macro

Learn more about using the [front panel interface](#)

Macro Example

The following is an example Visual Basic Scripting (vbs) program that you can copy, install, and run on your PNA

Note: Print these instructions if viewing in the analyzer. This topic will be covered by the Macro Setup dialog box.

1. Copy the following code into a [Notepad](#) file.
2. Save the file on the analyzer hard drive in the **C:\Documents** folder. Name the file **FilterTest.vbs**
3. Close Notepad
4. [Setup the macro in the PNA](#)
5. [Run the macro](#)

```
'Start copying here  
'This program creates a S21 measurement, with Bandwidth
```

```

'markers for testing a 175MHz Bandpass filter
'It is written in VBscript using COM commands

Set PNA = CreateObject("AgilentPNA835x.Application")
PNA.Preset
Set chan=PNA.activechannel
Set meas=PNA.activemeasurement
Set limts = meas.LimitTest
Set trce = PNA.ActiveNAWindow.ActiveTrace

meas.ChangeParameter "S21",1
chan.StartFrequency = 45e6
chan.StopFrequency = 500e6
trce.ReferencePosition = 8
PNA.TriggerSignal = 3

'Do Test
for t=1 to 5
call measure
call compare
next
msgbox("Done Testing")

sub measure
msgbox("Connect Device " & t & " and press OK")
PNA.ManualTrigger True
meas.SearchFilterBandwidth
end sub

sub compare
BW = meas.FilterBW
if bw>6.5e7 then msgbox("Failed BW: " & BW)
Loss = meas.FilterLoss
if loss>5 then msgbox("Failed Loss: " & Loss)
end sub
'End copying here

```

Calibration Overview

The following is discussed in this topic:

[What Is Measurement Calibration?](#)

[Why Is Calibration Necessary?](#)

[Conditions Where Calibration Is Suggested](#)

[What Is ECal?](#)

[See other Calibration Topics](#)

What Is Measurement Calibration?

Calibration removes one or more of the systematic errors using an equation called an error model. Measurement of high quality standards (for example, a short, open, load, and thru) allows the analyzer to solve for the error terms in the error model. See [Measurement Errors](#).


You can choose from different calibration types, depending on the measurement you are making and the level of accuracy you need for the measurement. See [Select a Calibration Type](#).

The accuracy of the calibrated measurements is dependent on the quality of the standards in the calibration kit and how accurately the standards are modeled (defined) in the calibration kit definition file. The calibration-kit definition file is stored in the analyzer. In order to make accurate measurements, the calibration-kit definition must match the actual calibration kit used. To learn more, see [Accurate Calibrations](#).

Calibration Wizard provides the different calibration methods used in the PNA. See [Calibration Wizard](#).

There are quick checks you can do to ensure your measurement calibration is accurate. To learn more see [Validity of a Measurement Calibration](#)

If you make your own custom-built calibration standards (for example, during in-fixture measurements), then you must characterize the calibration standards and enter the definitions into a user modified calibration-kit file. For more information on modifying calibration kit files, see [Calibration Standards](#).

 **Note:** [Instrument Calibration](#) is ensuring the analyzer hardware is performing as specified. This is not the same as measurement calibration.

Why Is Calibration Necessary?

It is impossible to make perfect hardware that would not need any form of [error correction](#). Even making the hardware good enough to eliminate the need for error correction for most devices would be extremely expensive.

The accuracy of network analysis is greatly influenced by factors external to the network analyzer. Components of the measurement setup, such as interconnecting cables and adapters, introduce variations in magnitude and [phase](#) that can mask the actual response of the device under test.

The best balance is to make the hardware as good as practically possible, balancing performance and cost. Calibration is then a very useful tool to improve measurement accuracy.

Conditions Where Calibration Is Suggested

Generally, you should calibrate for making a measurement under the following circumstances:

- You want the best accuracy possible.
- You are adapting to a different connector type or impedance.
- You are connecting a cable between the test device and an analyzer test port.
- You are measuring across a wide frequency span or an electrically long device.
- You are connecting an attenuator or other such device on the input or output of the test device.

If your test setup meets any of the conditions above, the following system characteristics may be affected:

- Amplitude at device input
- Frequency response accuracy
- Directivity
- Crosstalk (isolation)
- Source match
- Load match

What Is ECal

ECal is a complete solid-state calibration solution. It makes one port (Reflection), full two and three-port calibrations fast and easy. See Using ECal.

- It is less prone to operator error.
- The various standards (located inside the calibration module) never wear out because they are switched with PIN-diode or FET switches.
- The calibration modules are characterized using a TRL-calibrated network analyzer.
- ECal is not as accurate as a good TRL calibration.

For information about ordering ECal modules, see Analyzer Accessories or contact your Agilent Support Representative

Select a Calibration Type

This section provides information about the calibration types available in the PNA.

Calibration Types

[OPEN / SHORT Response](#)

[Full SOLT 2-port](#)

[THRU Response \(Isolation Optional\)](#)

[Full TRL 2-port](#)

[1-PORT Reflection](#)

[Full SOLT 3 or 4-port](#)

Learn about applying [FCA Cal Types](#).

See other Calibration Topics

Type: **Open and Short Response**

Calibration Method: [Unguided Calibration](#)

General Accuracy: Low to Medium

Parameters: S11 or S22 (S33 on a 3-port PNA)

Standards Required: OPEN or SHORT

Systematic Errors Corrected:


Frequency response reflection tracking

Application:

Reflection measurements on any one port.

Type: **Thru Response (Isolation Optional)**

Calibration Method: [Unguided Calibration](#)

 General Accuracy: Medium

Parameters: Transmission measurements

Standards Required: THRU

Isolation: One LOAD for each PNA test port.

Systematic Errors Corrected:

- Frequency response transmission tracking
- Crosstalk

Applications:

- Transmission measurements in any one direction.
- Isolation improves high dynamic range measurements. Learn more about [Isolation](#)

Note: The THRU definition for a predefined calibration kit assumes zero-length and zero-loss. If you use an adapter as a THRU, characterize the adapter in the calibration kit file for better accuracy. See [Accurate Calibrations](#)

Type: **1-Port (Reflection)**

Calibration Method: Unguided Calibration, Guided Calibration, ECal

General Accuracy: High

Parameters: Reflection measurements (S11 or S22 or S33 or S44)

Standards Required: (SHORT, OPEN, LOAD) or ECal module

Systematic Errors Corrected:

- Directivity
 - Source match
 - Frequency response reflection tracking
-

Application:

- Reflection measurements on any one port.
-

PNA Models: All

Type: **Full SOLT 2-Port**

General Accuracy: High

Calibration Method: Unguided Calibration, Guided Calibration, ECal

Parameters: All

Standards Required: (SHORT, OPEN, LOAD, THRU) or ECal module

Systematic Errors Corrected:

- Directivity
 - Source match
 - Isolation
 - Load match
 - Frequency response transmission tracking
 - Frequency response reflection tracking
-

Application:

- Use for all S-parameter measurements.
 - 12-term error-correction
-

Type: **Full TRL 2-Port**

Only on PNA Models E8356A, E8357A, E8358A, E8362A, E8363A, E8364A

Calibration Method: Unguided Calibration

General Accuracy: Very High

Parameters: All

Standards Required: THRU, REFLECT, LINE

Systematic Errors Corrected:

- Directivity
 - Source match
 - Isolation
 - Load match
 - Frequency response transmission tracking
 - Frequency response reflection tracking
-

Application:

- Use for all S-parameter measurements.
 - 12-term error-correction
 - Highest accuracy of all calibrations
-

For more information, see TRL Cal

To perform a TRL calibration with a connector type other than 3.5 mm or 7 mm, you must first modify or create TRL standards and definitions. For more information on modifying standards, see Calibration Standards.

Type: **Full SOLT 3 or 4-Port**

3-Port: Only on PNA Models N3381A, N3382A, N3383A, N5230A opts 240 / 245

4-Port: Only on PNA Models N5230A opts 240 / 245

General Accuracy: High

Calibration Method: Guided, ECal

Parameters: All

Standards Required: (SHORT, OPEN, LOAD, THRU) or ECal module

Systematic Errors Corrected:

- Directivity
 - Source match
 - Isolation
 - Load match
 - Frequency response transmission tracking
 - Frequency response reflection tracking
-

Application:

- Use for all S-parameter measurements.
-

Calibration Wizard

The Calibration Wizard allows you to choose a Calibration method and then perform the calibration.

How to Start Calibration Wizard

Guided Calibration: Mechanical Standards

Unguided Calibration

Saving a Calibration

Calibration Preferences


Other Cal Topics

How to start Calibration Wizard

Use one of the following methods:

-  + 
-  + 
- 

Learn more about using the [front panel interface](#)

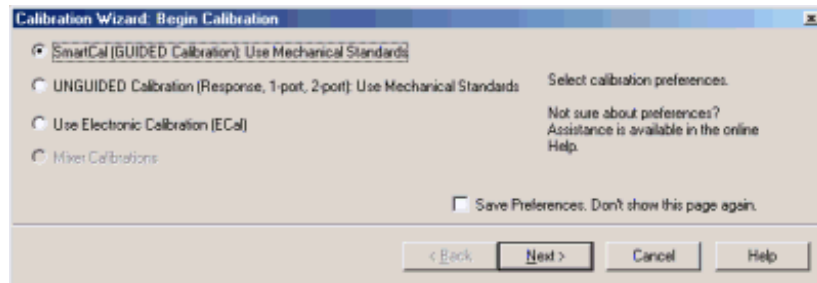

Calibration Wizard dialog box help

Allows you to select the calibration method:

SmartCal (Guided Calibration Use Mechanical Standards)

This method provides a step-by-step "wizard" interface. You describe the connectors on your DUT and the cal kits you will use; it walks you through the most accurate calibration possible.

- Supports all Cals EXCEPT simple response Cals (open, short, thru).
- Supports ECal on one or more ports, beginning with [PNA firmware revision 5.24](#).

Learn more about [SmartCal](#)

See Also [TRL Calibration](#)

Unguided Calibration Use Mechanical Standards

This method provides a familiar calibration interface. You choose the type of cal to perform; it allows you the flexibility to measure the standards in any order.

- Supports all Cals EXCEPT full 3-port, full 4-port, or TRL Cals.

Learn more about [Unguided Calibration](#)

Use Electronic Calibration

This method provides fast, software controlled calibrations.

See [Using ECal](#)

Mixer Calibration

This method is only available if the PNA has the [Frequency Converter Application \(option 083\)](#).

Save Preferences

When checked, saves your calibration method choice. You will not see this page again until you need to change the calibration method. To change, on the **Calibration** menu, click **Preferences**. When cleared, you will continue to see this page on subsequent calibrations.

SmartCal (Guided Calibration) Mechanical Standards

Depending on the DUT connector types you specify, the CAL WIZARD automatically determines the calibration type and suggests a calibration kit.

[Learn how to do TRL cals](#)

Note: To perform a Full 1-Port cal, select 'Not Used' for the unused DUT connectors.


The PNA displays the following dialog boxes when performing a Guided calibration:

[Select Guided Cal Type](#)

[Select DUT Connectors and Cal Kits](#)

Modify Cal Settings

Guided Calibration Steps

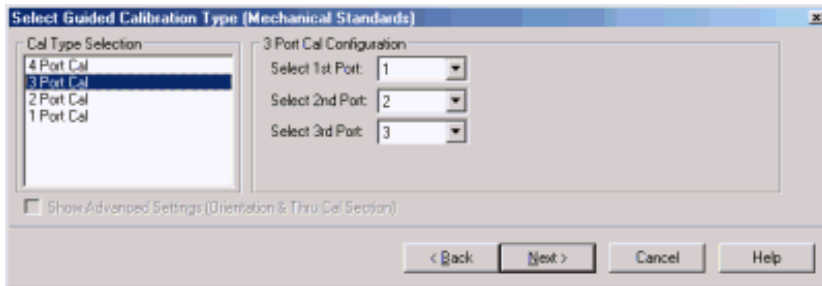


Select Guided Calibration Type dialog box help

Allows you to select calibration type and settings.

Cal Type Selection Select the type of calibration to perform.

Cal Configuration If not calibrating all PNA ports, specify which ports to calibrate.

Show Advanced Settings (Orientation & Thru Cal Section) Available only for ECal.

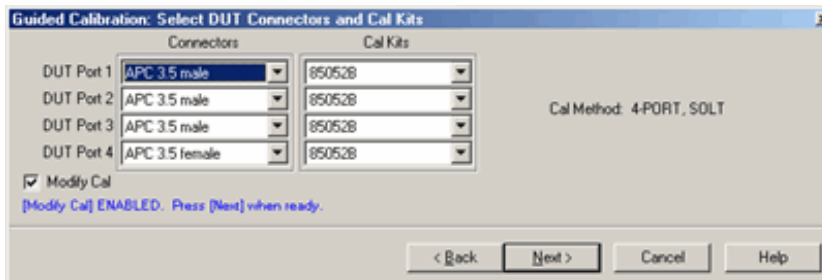

Select DUT Connectors and Cal Kits dialog box help

Allows you to select the connector type and Cal Kit for each DUT port to be calibrated.

Connectors


If your DUT connectors are:

- **Waveguide** Change the system impedance to 1 ohm before performing a calibration. See Setting System Impedance.
- **Not listed** (male and female) Select **Type A** as the connector type. Type A requires a calibration kit file containing the electrical properties of the standards used for calibration (see Calibration kits).
- **Unspecified** (like a packaged device) Select **Type B** as the connector type. Type B requires a calibration kit file containing the electrical properties of the standards used for calibration (see Calibration kits).
- **Non-insertable** Guided Cal will perform an Adapter Removal calibration. This requires that you have an adapter that has the same connectors as the DUT. To override this behavior, check Modify Cal or Modify Thru Method.

Cal Kits Select the Cal Kit to be used to calibrate each test port. The list for each DUT Port displays kits having the same connector type as the DUT.

Note: To perform a TRL Cal, assign a Cal Kit that contains TRL standards to the lowest port number of each port pair.

Modify Cal Check, then click Next, to Modify Cal (Standards AND Thru Method).

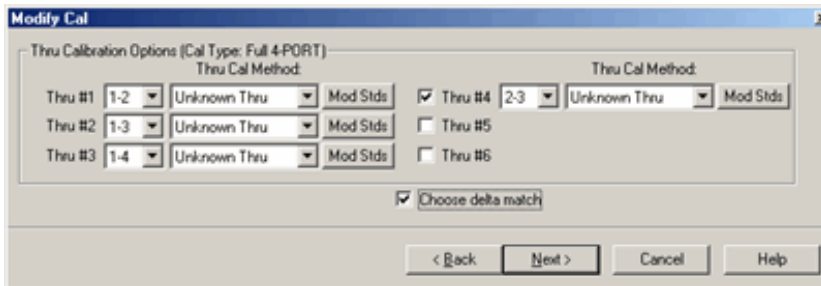

Modify Cal dialog box help

See ECal dialog box help.

Thru Calibration Options

Thru #n

Lists the proposed Thru connections to be made during the calibration process. You can change these Thru connections to better suit your test setup.

- The required Thru connection are listed without a checkbox to the left.
- The optional Thru connections can be selected for higher accuracy. See 4-port errors.

Thru Cal Method

Lists the available types of Thru Cal methods for the connectors on the specified port pairs.

Adapter Removal Learn more.

Cal Kit Thru (Defined Thru) Use a defined standard which exists in the selected Cal Kit with the same connectors as those for the two ports of the DUT. You must first use the Modify Cal Standards dialog box to define the THRU standard and add it to the Cal Kit. Learn more about Defined Thru.

Flush Thru Same as Zero-length THRU for insertable DUTs.


Unknown Thru Learn more.

Mod Stds Click to invoke the Preview and Modify Calibration Selections dialog box

Choose delta match Available when any Thru path involves an **Unknown Thru** or **TRL** cal on a PNA that does NOT have one reference receiver for each test port.

Check, then click **Next**, to invoke the Select Cal Set for Delta Match dialog box. Learn more about Delta Match Cal.

When cleared, the Cal Wizard attempts to use the current setup to perform a Delta Match Cal before completing the TRL or Unknown Thru Cal. If the current setup does not support the Delta Match Cal, the Select Cal Set for Delta Match dialog box appears.

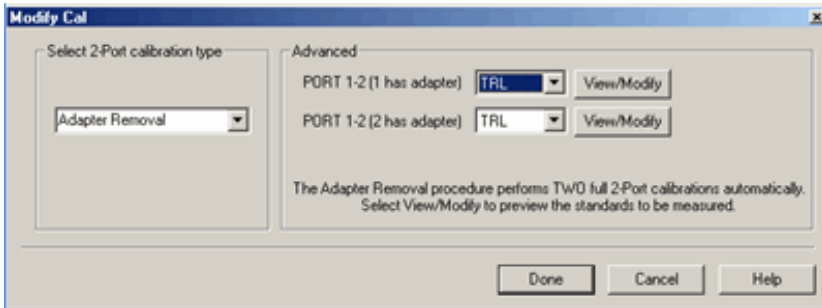

Modify Cal dialog box help

Select 2-port calibration type

Another chance to change the Thru method

Adapter Removal Learn more about [Adapter Removal](#).

Cal Kit Thru (Defined Thru) Use a defined standard which exists in the selected Cal Kit with the same connectors as those for the two ports of the DUT. You must first define the THRU standard and add it to the Cal Kit using [Modify Cal Standards](#). Learn more about [Defined Thru](#).


Flush Thru Same as [Zero-length THRU](#) for insertable DUTs.

Unknown Thru

Advanced

Select the cal method for each connector of the Thru pair. TRL is only available if a TRL cal kit was selected for the lowest port number of the port pair.

View Modify Click to invoke the [Preview and Modify Calibration Selections](#) dialog box.

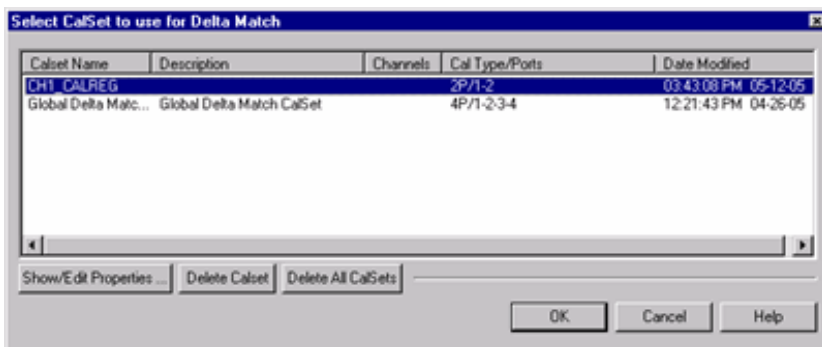


Select Cal Set for Delta Match dialog box help

Displays the Cal Sets that meet the requirements of the Delta Match Cal.

Select either a User Cal Set or Global Delta Match Cal.

If you have NO Cal Set to select:

1. Click **Cancel**, then **Cancel** again to quit the Cal Wizard.
2. Perform a Global Delta Match Cal.
3. Select Global Delta Match Cal when you re-calibrate and again see this dialog box.
4. When selected, it will probably be interpolated and the following dialog box appears.

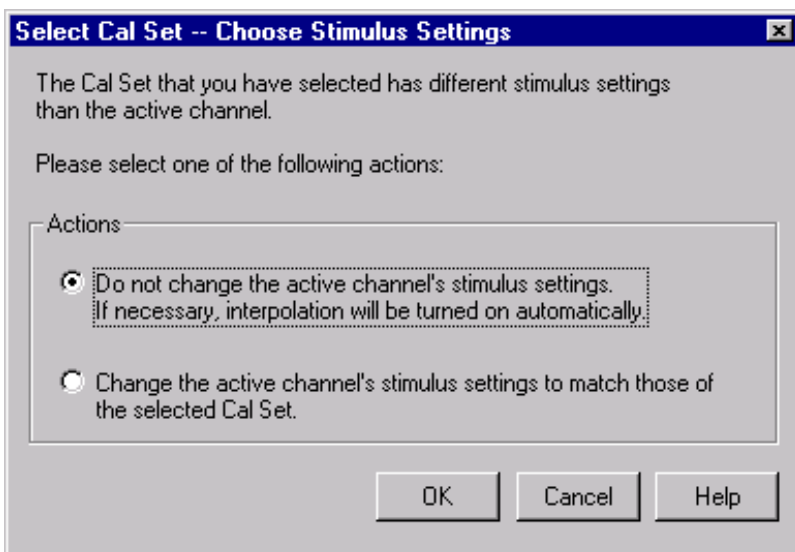


Select Cal Set -- Choose Stimulus Settings dialog box help

You have selected the Global Delta Match Cal to correct the delta match error terms. This Cal Set covers the full PNA frequency range and WILL need to be interpolated.

Select **Do not change...** then click **OK**.

Accuracy of the Delta match errors will NOT be degraded.

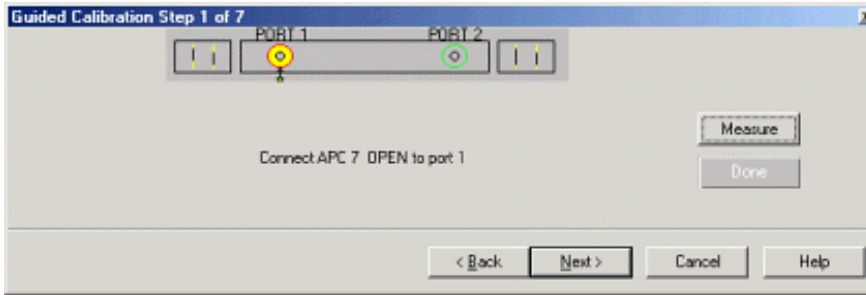

Calibration Steps dialog box help

Prompts for standards to be measured.

Measure Click to measure the standard.

Done Click **after** a standard is re-measured and all measurements for the calibration are complete.

Next Click to continue to the next calibration step. Does **NOT** measure the standard.

If a standard is NOT measured, a warning appears and **Done** will not be available after the last Cal step.

The Calibration Complete dialog box appears after all standards are measured.

Unguided Calibration

Unguided calibration does **NOT** support **Full 3-Port, 4-Port, or ECal** calibrations.

The PNA displays the following dialog boxes when performing an Unguided calibration:


Select Calibration Type for Mechanical Standards

Select Cal Kit

Measure Mechanical Standards

Multiple Standards

Sliding Load Measurement

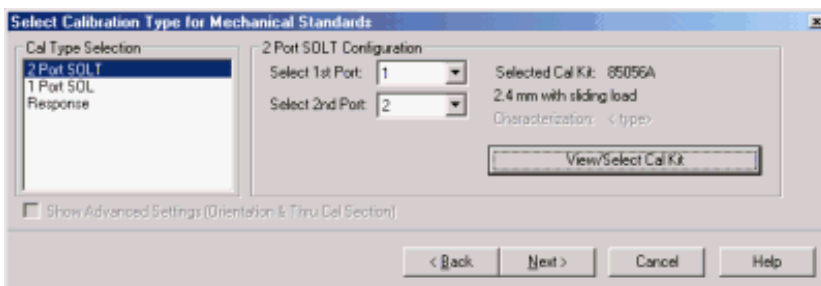

Select Calibration Type for Mechanical Standards dialog box help

Calibration Type Selection


- 2-Port SOLT
- 1-Port SOL
- **Response** - Reflection and Thru (if the active measurement is transmission)

Cal Configuration If not calibrating all PNA ports, specify which ports to calibrate.

View/Select Cal Kit Click to invoke the [Select Cal Kit dialog box](#).

Next Click to continue to [Measure Mechanical Standards](#) dialog box.

Note: If the DUT connector type has an impedance other than 50 ohms (waveguide = 1 ohm), change the system impedance before performing a calibration. See [Setting System Impedance](#).

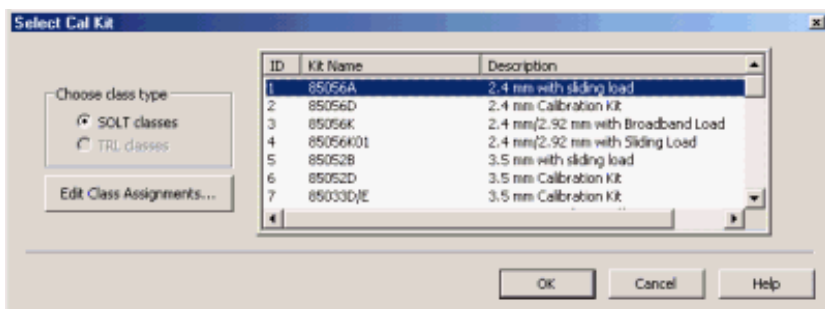

Select Cal Kit dialog box help

Displays the calibration kit files available for Unguided calibration.


Select the desired calibration kit file and click **Next**

Choose class type

TRL calibration is NOT available on the 4-port PNA because there is only 1 reference receiver.

Edit Class Assignments Allows modification of the selected Cal Kit class assignments.

To learn to substitute other calibration kits, see [Advanced Modify Cal Kits](#)

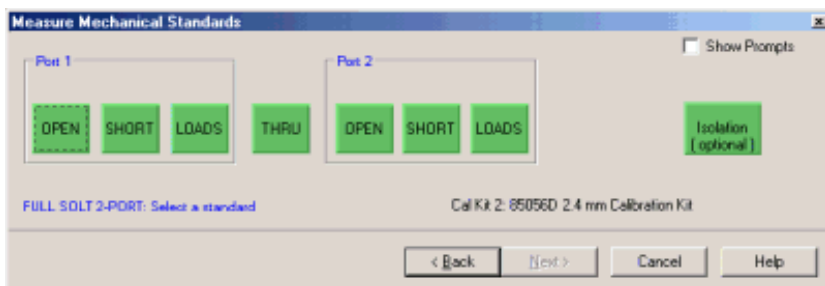


Measure Mechanical Standards dialog box help

Displays the calibration kit file and standards required for the calibration.

- Standards may be connected and measured in any order.
- Connect the standard to the measurement port and click its associated green button. A check mark indicates the standard has been measured.
- If a standard type contains multiple standards, the [Multiple Standards dialog box](#) opens to display the multiple standards included in the calibration kit file.
- If a sliding load is included in the calibration kit file, the [Sliding Load dialog box](#) opens to perform the measurement with the standard.
- **Reflection Response** Select EITHER Open or Short standard, then click Next.
- **Isolation** Requires one load for each test port of the PNA. [Learn more about Isolation](#). Use when your measurement requires maximum dynamic range (> 90 dB). See also [Isolation Portion of 2-Port Calibration](#).
- **Normalize** Available when performing a response cal for any measurement. After Normalize is pressed and the Cal is complete, the data trace is flat when the same physical connections are present on the port. This is similar to [Data/Memory](#), except that the response cal is [saved with Cal data](#) and can be applied to other like measurements. Data/Memory is still available after using Normalize. You would usually connect a THRU standard when calibrating a transmission measurement, and a SHORT standard when calibrating a reflection measurement.

Show Prompts Check to provide a reminder for the required connection when you click on the standard.

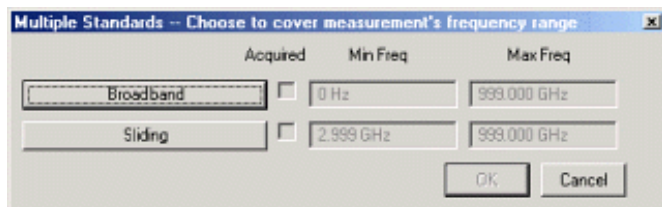

Multiple Standards dialog box help


Select the standards to be measured.

Note: You may see both male and female standards. The Unguided cal has no knowledge of the gender of your connector types. **Choose the gender of your DUT connector;** NOT the test port. Then click OK.

To modify this calibration class to show only one standard, on the Calibration menu, click **Advanced Modify Cal Kits**. Select the Cal kit and click **Edit Kit**. In **Class Assignment**, click **Edit**. Learn more about [Modify Calibration Class Assignments](#).

- Connect the standard to the measurement port and click its associated button. A check mark in the **Acquired** box indicates the standard has been measured.
- To cover the entire frequency range, you may need to measure more than one standard. The order in which the standards are measured is important. The last standard that is measured will override the others in respect to the frequency range of the standard definition. **Example:** In the case of measuring both a broadband load and a sliding load, you would measure the sliding load last. This is because the frequency range of the sliding load is a subset of the broadband load.

Learn more about [Modify Calibration Class Assignments](#)

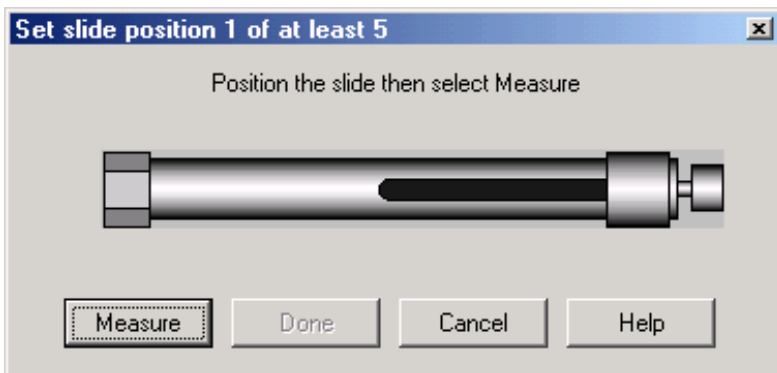

Sliding Load Measurement dialog box help

Allows you to measure the sliding load standard.

To Measure a Sliding Load:

1. Connect the sliding load to the measurement port.
2. Position the sliding element, then click **Measure**. Do not move the sliding element until measurement is complete.
3. Measure the sliding load for at least **five** and up to **seven** positions for best accuracy.


Note: The positions of the sliding element should cover the full length of the slide, but be unequally spaced to reduce the possibility of overlapping data points.

5. Click **Done** for final measurement.
6. Remove sliding load from the measurement port.

7. Measure the remaining standards.

Saving a Calibration

ECAL, Guided, and Unguided Calibrations end with the following dialog box:

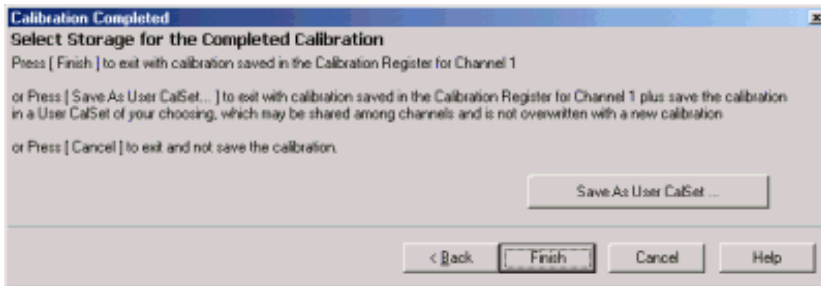

Calibration Completed dialog box help


Finish Save to the channel's calibration register.

Save As User Cal Set Invokes the [Save as User Cal Set dialog box](#) AND save to the channel's calibration register.

Cancel Calibration is NOT applied or saved.

Learn about [Calibration Registers](#).

Learn about [User Cal Sets](#)

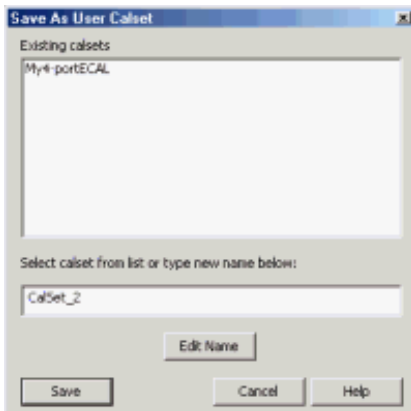

Save as User Cal Set dialog box help

Existing Cal Sets - Lists the Cal Set names saved on the PNA.

Select Cal Set from list or type new name below Specify a name for the new Cal Set. Either accept the suggested new name, type a new name, or select a name from the list to overwrite an existing name.


Edit Name If there is no keyboard, click to start the PNA typing tool that can be used from the PNA front panel.

Save Saves the Cal Set to the new Cal Set name.


Learn about [User Cal Sets](#)

Calibration Preferences

How to change Cal Preferences

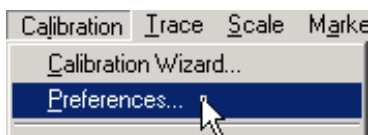

Learn more about using the [front panel interface](#)

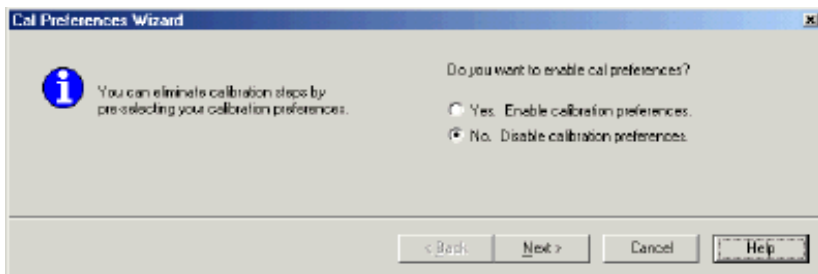

Cal Preferences dialog box help


Cal preferences allows you to save the following selections from the [Begin Calibration](#) page of the Cal Wizard:

- Cal method (Guided, UnGuided, ECal)
- Create New Cal Set (checked or cleared)

Yes. Enable calibration preferences The selections will always be made and you will not see the [Begin Calibration](#) page again until you disable calibration preferences. Click **Next** to make your selections on the Begin Calibration page.

No. Disable calibration preferences See the [Begin Calibration](#) page every time you start Cal Wizard. Click **Next** to see the following dialog box confirming your choice to disable preferences.

Note: You can also Enable calibration preferences directly from the [Begin Calibration](#) page.

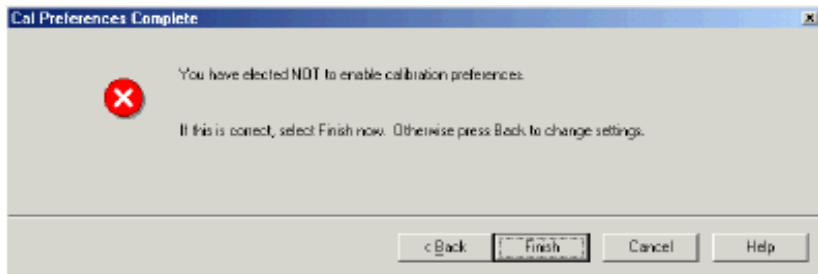

Cal Preferences Complete dialog box help

Click **Finish** to complete cal preferences.

Using Calibration Sets

Calibration Sets (Cal Sets) enable you to use a single calibration on multiple channels.

[What are PNA Cal Sets](#)

[Cal Registers and User Cal Sets](#)

[Managing and Applying Cal Sets](#)

[Examples of Cal Set Usage](#)

[Archiving Cal Sets using .cal files](#)

See other Calibration Topics

What are PNA Cal Sets

At the completion of a calibration, all calibration data is stored to a Cal Set. The Cal Set can be applied later to a different channel that has the same stimulus settings as the Cal Set, thereby saving the time it takes to perform another calibration. The following data is saved to a Cal Set:

- Name
- Cal Set Description
- Cal Set Attributes - stimulus settings, cal type, port association
- Standards data
- Error term data
- GUID (Global Unique Identifier)

Cal Registers and User Cal Sets

There are two types of Cal Sets:

- **Cal Registers** (channel specific)
- **User Cal Sets**

Calibration data is automatically saved to a Cal Register at the end of every calibration. You can also choose to save the cal data to a User Cal Set.

Calibration Registers

New with PNA Release 5.0, Calibration Registers are designed to simplify calibrations for most users. When a calibration is complete, the data is automatically saved to the channel's Cal Register, overwriting (or appended to) the previous cal data stored in that register. This concept is similar to previous Agilent Vector Network Analyzers.

- Every channel has ONE dedicated Cal Register. They are named CHn_CALREG, where **n** is the channel

number. The name cannot be changed.

- Cal Registers are more volatile because they are overwritten (or appended) each time a calibration is performed on that channel. The Cal data is always saved, but only temporarily.
- Cal Registers can be applied to other measurements, but ONLY on the same channel as the Cal Register.

User Cal Sets

At the end of a calibration, you can choose to also save cal data to an existing or new User Cal Set.

- User Cal Sets can be applied to any number of channels simultaneously.
- User Cal Sets are named by you for easy identification.
- You can have an unlimited number of User Cal Sets.
- All User Cal Sets reside in a single file (PNACalSets.dat) on the PNA.
- At any time, you can copy Cal Register data to create a User Cal Set. See Cal Set Properties.

Appending Data in a Cal Set

At the end of a calibration, data is saved to the channel's Cal Register and, if you choose, to an existing User Cal Set. The PNA attempts to append new error terms to a non-empty Cal Set. The existing Cal Set data is completely overwritten UNLESS the new data can coexist with the existing data according to the following two rules:

- The stimulus settings of the new data must exactly match the existing data.
- The new cal must involve different ports from the existing cal.

For example:

Case 1 - An existing Cal Set contains a full 2-port cal between ports 1 and 2. Using the same stimulus settings, you perform a 1-port cal on port 3. At the end of the cal, you click Save As User Cal Set and select the existing full 2-port User Cal Set.

Result: The 1-port cal is appended to the 2-port User Cal Set. There is NO overlap between them.

Case 2 - Same situation as Case 1, except the 1-port cal is performed on port 1.

Result: The Cal Set will contain a 1 port cal on port1 and a 1 port cal on port 2. The overlapping tracking terms are removed rendering the original full 2 port cal invalid.

Managing and Applying Cal Sets

The PNA attempts to apply a Cal Set, and turn error correction ON, for ALL of the measurements on the active channel. This may not always be possible. For example, suppose a channel contains both S11 (reflection) and S21 (transmission) measurements. If a Cal Set that contains only an S11 **Cal Type** is applied to that channel, the Cal Set does not contain the error terms to correct the S21 measurement. Error correction is turned ON for the S11 measurement and NOT turned on for the S21 measurement.

There are two ways to apply an existing Cal Set (Cal Register or User Cal Set) to a measurement:


1. Recalling an Instrument State with Cal data (.cst file) - A .cst file contains an Instrument State with all measurement attributes AND a 'pointer' to the Cal Set that was used to calibrate the measurement.

NOTE: Before saving a .cst file, be sure that a User Cal Set (NOT a Cal Register) is being used for the


measurement. Because Cal Registers are automatically overwritten when a new calibration is performed, it is likely that the Cal Register data will change before the .cst file is recalled.

2. Create a new measurement and select a Cal Set to apply to the active channel.

How to Select and Apply a Cal Set to the active channel

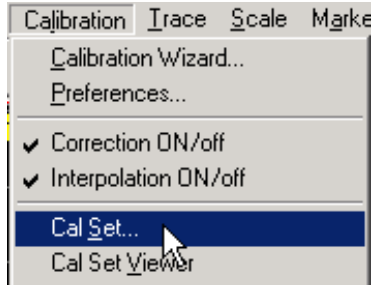

Learn more about using the [front panel interface](#).

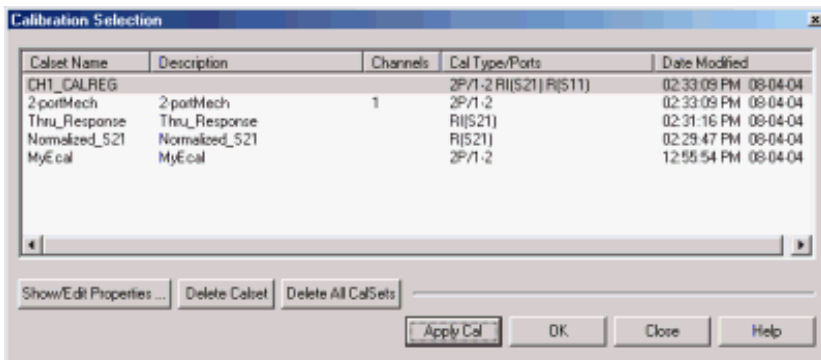

Calibration Selection dialog box help

This dialog box allows you to manage and apply Cal Sets.

Although the number of Cal Sets you can have is limited only by the amount of PNA memory, it is considered unusual to have more than about 10 existing Cal Sets, or one current Cal Set for every unique channel setup. Old Cal Sets (with 'stale' data) should be deleted or overwritten.

Note: The active channel's Cal Register always appears, even if empty. Cal Registers that belong to other channels appear in the list of Cal Sets only if the channel exists, and only if they contain data.

- Learn about [Cal Registers](#).
- Learn how to [View the Error Terms of a Cal Set](#).

Click a row to select that Cal Set.

Columns click a heading to sort by that column

Cal Set Name Name to identify the Cal Set.

Description User-settable text to further identify the Cal Set.

Channels Channel numbers that are currently using this Cal Set. A blank entry means it is not currently in use.

CalType / Ports Type of Cal contained in the Cal Set. [Learn about applying appropriate Cal Types](#).

Cal Type Abbreviations:

1P, 2P, 3P, 4P - Full n-Port calibrations

R - Response (instead of ports, shows the measurement type that it corrects.)

Modified Date and time the Cal Set was last modified.

Buttons

Show / Edit Properties Invokes the Cal Set Properties dialog box. This allows you to view all of the Cal Set properties and create a **duplicate** User Cal Set from an existing User Cal Set or Cal Register.

Delete Permanently deletes the Cal Set after you choose OK to a warning prompt.


Delete All Permanently deletes ALL listed Cal Sets and Cal Registers after you choose OK to a warning prompt.

Apply Cal Applies a Cal Set to the active channel. If the stimulus settings of the Cal Set and channel are different, a choice must be made.

Unselect If the selected Cal Set is being used by a channel, this button 'Un-applies' a Cal Set from the active measurement.

OK Applies the selected Cal Set and closes the dialog box.

Close Exit the dialog box without selecting a Cal Set.

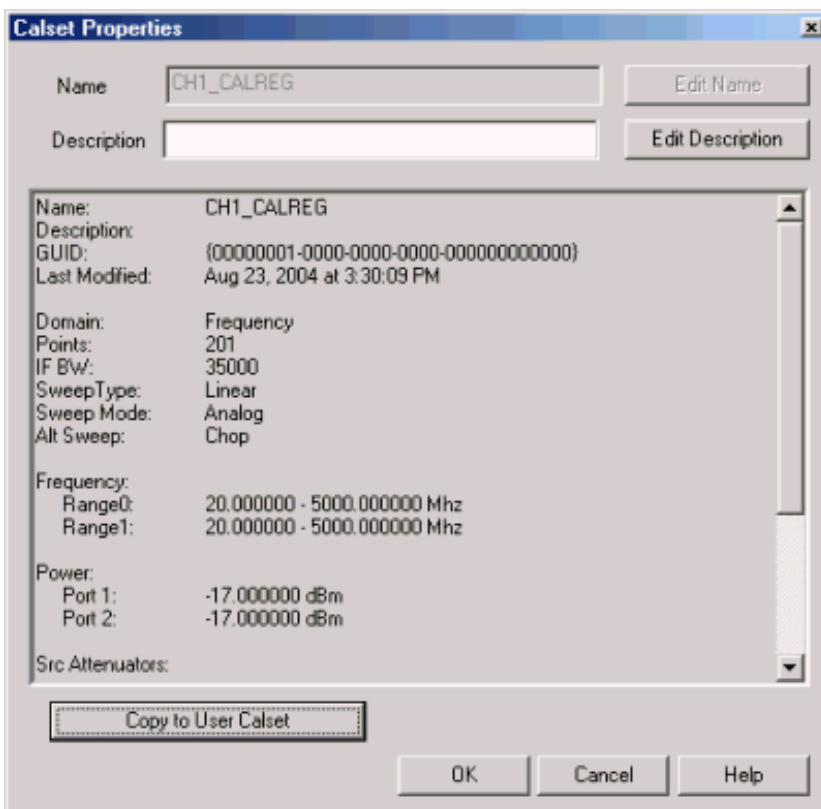

Cal Set Properties dialog box help

Allows you to view all of the Cal Set properties and create a **duplicate** User Cal Set from an existing User Cal Set or Cal Register.

Columns click a heading to sort by that column

Name Edit name of the User Cal Set. You can NOT change the name of a Cal Register.

Description Descriptive text to further identify the Cal Set.

Cal Set Properties Lists descriptive information and stimulus conditions of the Cal Set. Learn how to [View the Error Terms of a Cal Set](#).

Copy to User Cal Set Invokes the [Save as User Cal Set](#) dialog box. Type a name for the copy of the selected Cal Set data.


Stimulus Setting Different between Cal Set and Measurement

The Cal Set contains the measurement settings that were used at the time of the calibration. These settings may be different than those of the new measurement to which the Cal Set is being applied. If there is a difference, you can choose between the following options.


- If the frequency span of the **Cal Set is equal to or greater than the measurement:**

Frequency Range

Cal Set |-----|
Measurement |-----|

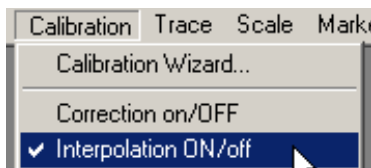

- **AND** Calibration, Interpolation is ON
 - Then choose **A**, **B**, or **Cancel**.
 - If Interpolation is OFF, **A** is not available.

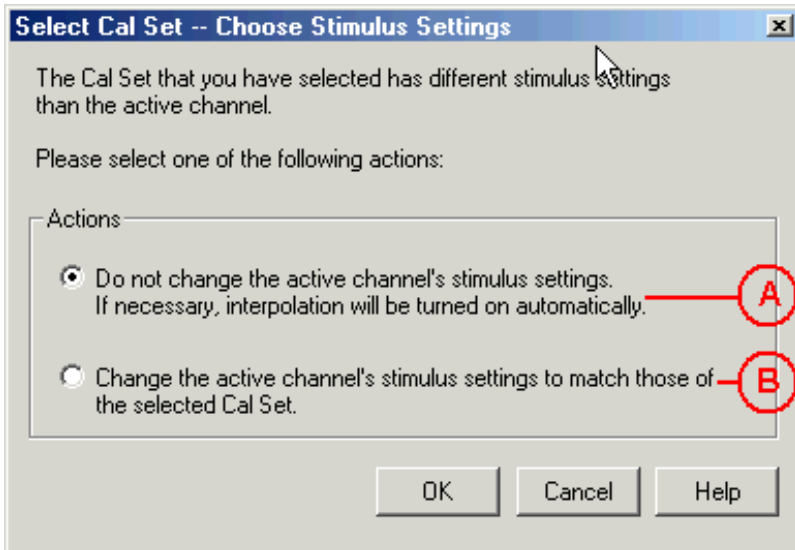


A The calibration will be interpolated if necessary. Learn more about [Interpolation Accuracy](#)


B The stimulus settings will change to equal the Cal Set.

Cancel Do NOT apply the Cal Set.

- If the frequency span of the **Cal Set** is less than the measurement:

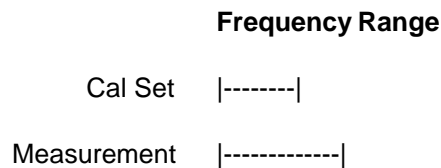

- OR, if Calibration Interpolation is OFF, then choose:

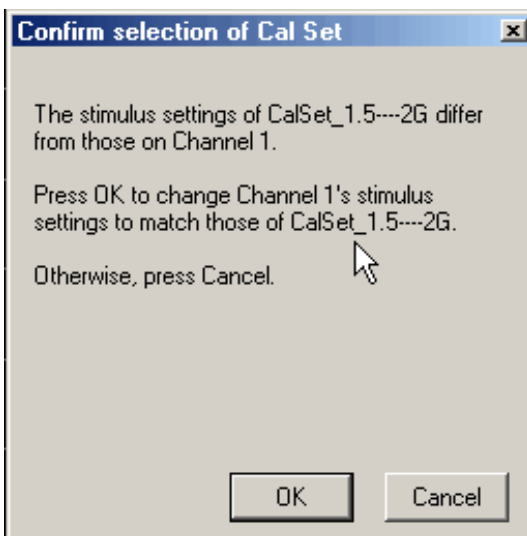

OK Reduce the measurement frequency span.

Cancel Cal Set will NOT be applied.

Examples of Cal Set Usage

The following examples show how Cal Sets increase flexibility and speed in making analyzer measurements.

Using one User Cal Set with many Channels

Using one Measurement with many Cal Sets

Using one User Cal Set with many Channels


It is possible to do one calibration, then apply it to several channels.

An example:

During a manufacturing process, you may have many calibrated channels. You may wish to continuously cycle through the measurements and examine them individually. Occasionally, you may wish to refresh the calibration without having to recreate all the measurement state files.

Here is how: Examine the stimulus settings for each channel. Then make the User Cal Set stimulus range a super-set of the whole group. Each channel can then use the same User Cal Set. Some calibrations will be interpolated. **Note:** Make sure that interpolation is turned on.

Notice in the following image, Cal Set 78 is used on more than one channel, in this case Channel 5 and 16 .

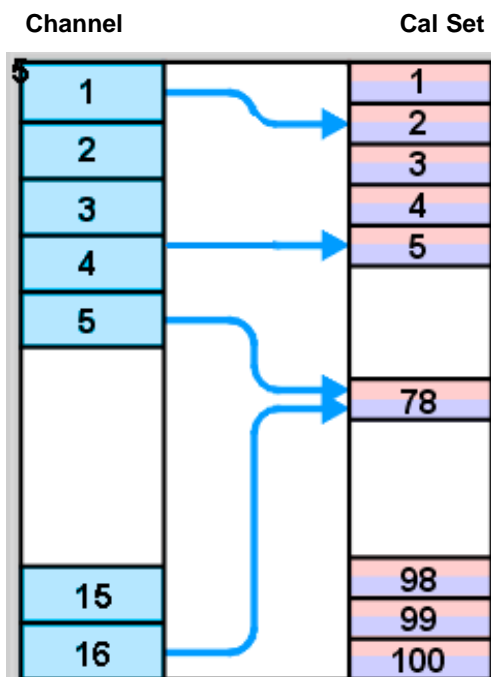

Using one Measurement with many Cal Sets

The drawback with having one very large User Cal Set associated with many instrument states could be a loss of accuracy due to interpolation. In such cases, consider using one User Cal Set for each stimulus setting. The stimulus conditions can then be changed for a channel by applying different User Cal Sets. Other settings (window setups, measurement definitions, scaling, limits, markers) will not change. This may result in faster state changes than if you saved and recalled *.cst files for each set of stimulus conditions.

Example #1: An amplifier needs to be measured at several input power levels. Calibrate at several power levels and save each calibration in a separate User Cal Set. Then, apply the User Cal Sets to the single measurement consecutively.

Example #2: Making an S21 Measurement, you need to measure both wide span and narrow span characteristics of the device. One Cal Set covers the wide span setup; another the narrow span setup.

Archiving Cal Sets using .cal files

Because User Cal Sets can easily be deleted, provide extra backup by also saving your calibration as a .cal file (see saving a .cal file).

Example:

One person performs a calibration, names and saves it as a User Cal Set. This Cal Set is available for any other person to use. A second user could accidentally delete or modify the User Cal Set requiring the originator to repeat the calibration.

Security can be provided for calibration data by saving the Cal Set to a **.cal** file. At a later time, the .cal file could be recalled and the original calibration restored.

Using ECal

This topic discusses all aspects of ECal:

[ECal Overview](#)

[Connect ECal Module to the PNA](#)

[Perform a Calibration Using ECal](#)

See Also:

[ECal User-Characterization](#)

[Restore ECal Module Memory](#)

[See other Calibration Topics](#)

ECal Overview

ECal is a complete solid-state calibration solution. Every ECal module contains electronic standards that are automatically switched into position during a PNA measurement calibration. These electronic standards have been measured at the factory and the data stored within the memory of the ECal module. The PNA uses this stored data, along with the PNA-measured data, to calculate the error terms for a measurement calibration.

ECal modules are available in 2-port and 4-port models and a variety of connector types, covering many frequency ranges. See [Analyzer Accessories](#) for more about available ECal modules and ordering information.

You can perform the following calibrations with ECal:

- 1-Port Reflection calibration
- Full 2-Port calibration
- Full 3-Port calibration
- Full 4-Port calibration

You can verify the validity of a mechanical or ECal calibration with [ECal confidence check](#).

Care and Handling of ECal Modules

You can improve accuracy, repeatability, and avoid costly repair of equipment in the following ways.

- Practice proper connector care. See [Connector Care](#).
- Protect equipment against ESD damage. Read [Electrostatic Discharge Protection](#).
- Do not apply excess power to ports. Refer to specifications provided with your ECal module.


Connect ECal Module to the PNA

ECal modules are controlled and powered through a USB connection to the PNA. When you connect the module, the PNA automatically recognizes the type of module, frequency range, and connector type.

Note: Certain USB devices (such as ECal modules) require you be logged on with Administrator privileges the first time you plug them into the PNA. This must be done for each serial number.

ECal modules connect to the USB port on the front or rear panel of the PNA.

1. Wear a grounded wrist strap when making connections.
2. Connect the USB cable **Type B** connector to the ECal module and the USB cable **Type A** connector to the front or rear panel USB connector of the analyzer, as shown in the following graphics.

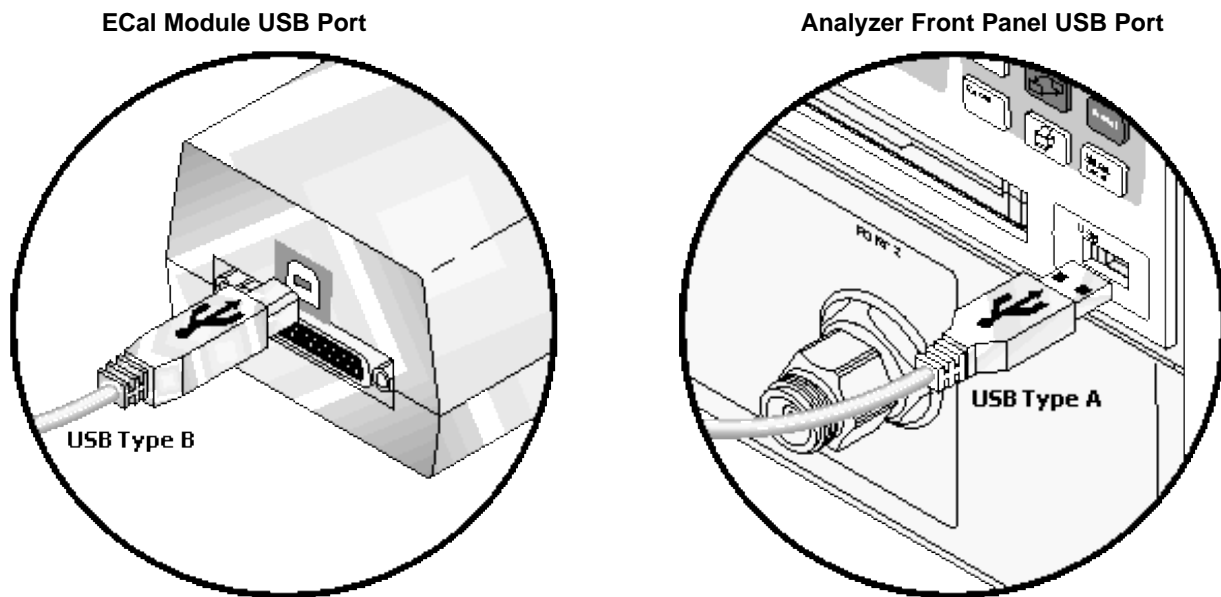

Notes:

- Agilent 8509x and N4431 ECal modules, when first connected, draw significantly more current than other modules. This could cause the USB to stop working in certain situations. See USB limitations.
- Unused ECal modules that have completed a calibration may remain connected to the USB port.
- You can connect and disconnect the ECal module while the analyzer is operating. However, **DO NOT** connect or disconnect the module while data transfer is in progress. This can result in damage or at least corrupted data.
- A USB hub may be used to connect more than one USB device to the analyzer. See Analyzer Accessories for more information about USB peripheral equipment.



ECal module not found dialog box help

Displays an error message indicating the ECal module is not connected or has not been recognized by the network analyzer.

Retry Check the USB connections and click to continue.

Notes:

- When the ECal module is connected to the network analyzer for the first time, it may take approximately 30 seconds for the analyzer to recognize the module and make it available for calibration.
- For best accuracy, allow the ECal module to warm-up until it indicates READY.
- See [Connect ECal Module USB to PNA USB](#).


Perform a Calibration Using ECal

Select an ECal module that has connectors of the same type and gender as the DUT. If such an ECal module is not available, a module with connectors different from the DUT can be used by using [Advanced Settings](#) or [User Characterization](#).


Connect the ECal module ports to the PNA ports. During the calibration process the PNA can either automatically detect how the ECal module is connected, or the orientation can be performed manually.

Note: Terminate any unused ECal ports with a 50 ohm load.

1. Connect the ECal module USB cable to the analyzer USB. See [Connect ECal Module USB to PNA USB](#).
2. Allow the module to warm up until it indicates **READY**.
3. Enter the analyzer settings. See [Set Up Measurements](#).
4. Start the [Calibration Wizard](#) as follows:

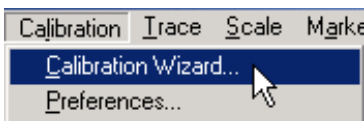

5. In the [Calibration Wizard](#) dialog box, click **Use Electronic Cal (ECal)**

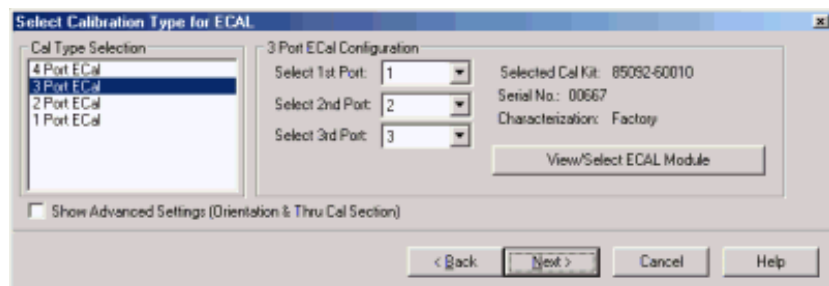

Select Calibration Type for ECal dialog box help

Allows you to select calibration type and settings.

Cal Type Selection / Configuration Select the number of ports to calibrate. Then select the port number configuration.

4 Port ECal Available only if using a 4-port PNA. No additional configuration necessary.

3 Port ECal Available only if using a 4-port or 3-port PNA.


2 Port ECal

1 Port ECal- (Reflection) Advanced Settings are not available.

View/Select ECal Module Click to [Select the ECal module](#) if more than one ECal module is connected to the PNA. Also, [Select the User Characterization](#) within the module. Learn more about [User Characterization](#).


Show Advanced Settings Check to display the [Advanced Settings](#) when **Next** is clicked.

Note: The PNA no longer allows ECal isolation to be performed. The inherent isolation of the PNA is better than that attained with correction using an ECal module.

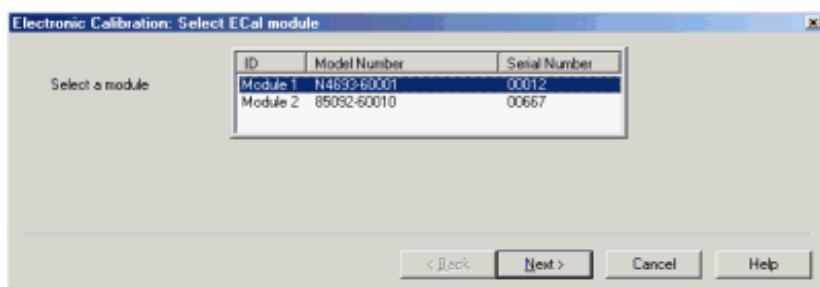


Select ECal Module dialog box help

If the PNA detects more than one ECal module, select one of the modules, then click **Next**.

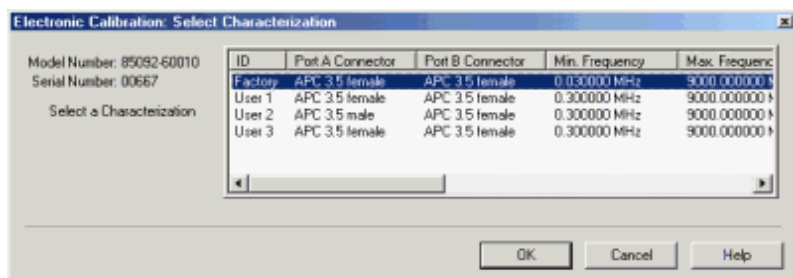

Select Characterization dialog box help

Select either the Factory Characterization of your ECal module or a [User Characterization](#). Once selected, that characterization becomes the default selection until the PNA is turned OFF and restarted. When restarted, **Factory** again becomes the default selection.

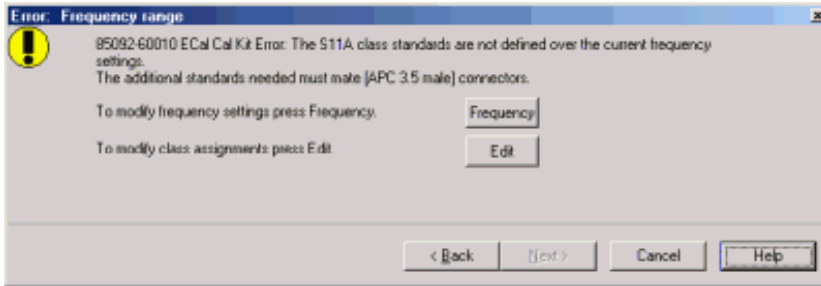

Error: Frequency Range dialog box help


The current cal standards (or ECal module) does not cover the current frequency range of the measurement. Do one of the following to correct the problem:

Frequency Reduce the frequency range of the active channel.

Edit This selection is not relevant to ECal modules.

Back Select a different characterization that covers the required frequency range.

Cancel Re-characterize the module with an increased frequency range.

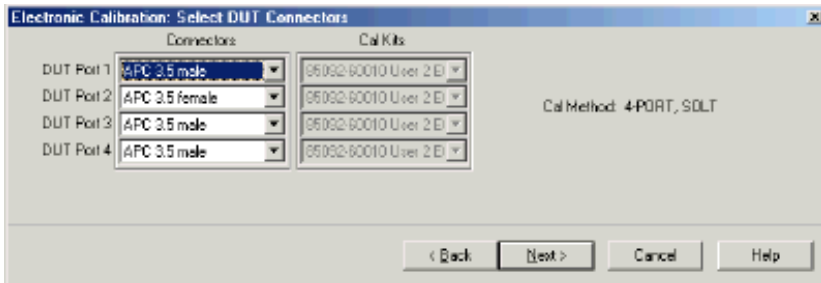


Select DUT Connectors and Cal Kits dialog box help

If the ECal module or selected User Characterization has more than one connector type, then the following dialog box is presented which allows you to change the DUT connector type. Otherwise, click next to proceed to Advanced Settings (if checked) or ECal Steps.

Connectors

The available connectors are listed for each DUT port.

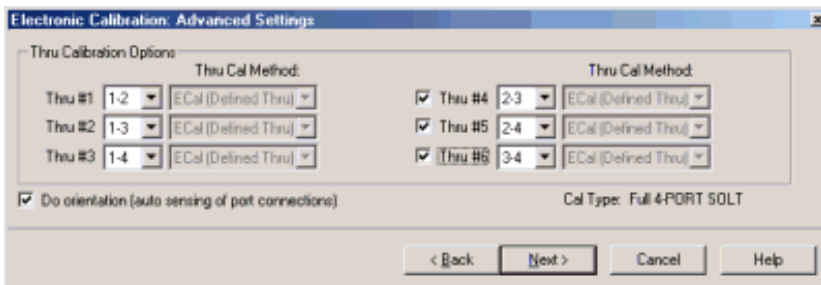

Advanced Settings dialog box help

Some settings are limited by the PNA model or ECal module connectors.

Thru Calibration Options

On a Full 4-Port SOLT calibration, you can choose to measure up to SIX THRU connections. The more THRU connections you measure, the better the accuracy of the calibration.

The following requires that you understand the terms "insertable and non-insertable" devices. See [Calibration Thru Methods](#) to learn about these terms.

Insertable Choices


ECal (Defined Thru) Measures the THRU state of the ECal module. The easiest selection for a 4-port PNA, but not as accurate as Flush Thru.

Flush Thru (zero-length Thru) The THRU state of the ECal module has more loss than a zero-length thru, resulting in degraded transmission tracking error terms. This setting requires an insertable ECal module. When this setting is checked, you will be prompted to remove the ECal module and connect the two reference planes directly together for a zero-length thru.

Non-Insertable Choice

Adapter Removal Can be used with ECal when your DUT is NON-insertable. However, the ECal module MUST be insertable, and the adapter connectors must exactly match the connectors of the DUT as in the following diagram.


Note: With PNA release 4.8, adapter removal now performs 2-port measurements on both sides of the adapter. It previously performed 2-port measurements on one side and 1-port measurements on the other. This improves the accuracy of the adapter removal calibration.

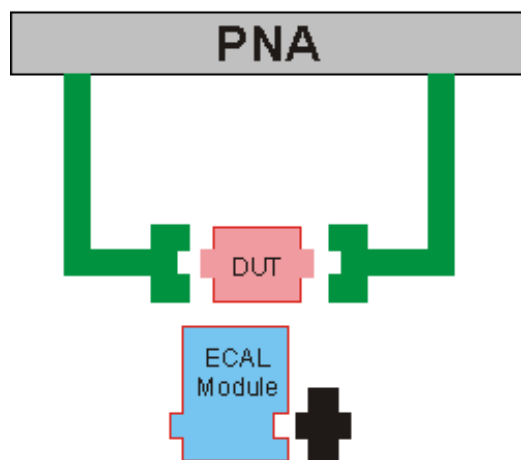

In cases when adapter removal cannot be performed, ECal [User Characterization](#) is ALWAYS possible if you have the right adapters. A User Characterization is performed once and stored in the ECal module. However, accuracy is compromised every time you remove, then reconnect, the adapter with the ECal module.


Do orientation When this box is checked (default) the PNA senses the model and direction in which an ECal module port is connected to the PNA ports. If power to the ECal module is too low, it will appear as if there is no ECal module connected. If you use low power and are having this problem, clear this check box to provide the orientation manually.

Orientation occurs first at the middle of the frequency range that you are calibrating. If a signal is not detected, it tries again at the lowest frequency in the range. If you have an **E8361A** or **E836xB** PNA and do an ECal completely within 10 - 20 MHz OR 60 - 67 GHz, you may need to do orientation manually. There may not be sufficient power to orient the ECal module at those frequencies.

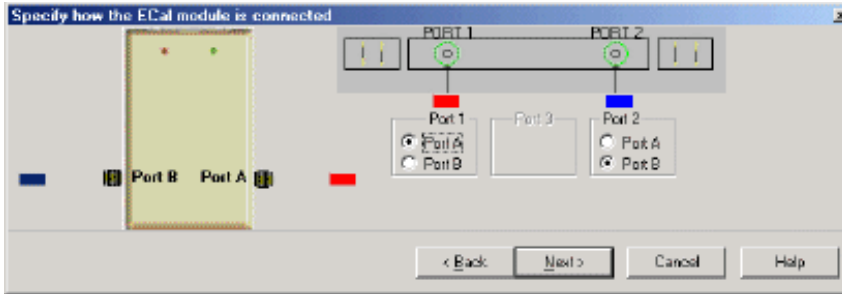

Specify how the ECal module is connected dialog box help

This dialog box appears when the **Do orientation** checkbox in the previous dialog box is cleared. Click Port A and B to reflect the orientation of the ECal module.

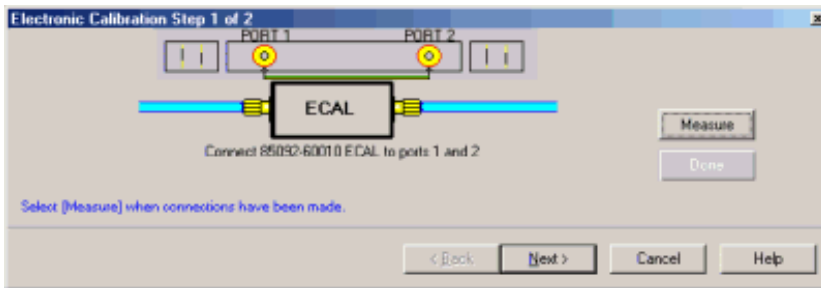

Electronic Calibration Steps dialog box help

Displays the instructions for each measurement required for calibration.

Measure Measures the ECal standards.

Done Click when last standard has been measured.

Saving a ECal Calibration

When complete, you can save the new calibration. [Learn how.](#)

ECal User Characterization

[Overview](#)

[How to Perform a User Characterization](#)

[Restore ECal Module Memory](#)

See also [Using ECal](#)

Other Calibration Topics

Overview

A user characterized ECal allows you to add adapters to the ECal module, re-measure the ECal standards INCLUDING the adapters, then add that data to ECal memory. This extends the reference plane from the module's test ports to the adapters.

There are several reasons you might want to perform a user characterization:

- If you need to use adapters with your ECal module, you could characterize your ECal module with the adapters attached and perform subsequent ECals with a single step.
- If you have a 4-port ECal module, you could configure the module with adapters of different connector types. Then perform a user characterization of the module. When you need to test a DUT with a pair of the connector types on your module, calibrate the PNA with a 1-step ECal using the two connectors of the User characterized module.
- If you test devices in a fixture, you could embed the characterization of the fixture in the characterization of the module. To do this, during the mechanical calibration portion of the user characterization, calibrate at the reference plane of the device as you would normally calibrate. Then remove the fixturing to be embedded and insert the ECal module to be characterized. When measuring the ECal module, the PNA removes the effects of the fixturing and stores the measurement results in the user characterized ECal module. Subsequent calibrations with that user characterized module will also remove the fixture effects.




Notes:

- User Characterization does not delete the factory characterization data. The factory data is saved in the ECal module in addition to the user characterization data.
- You can save up to five different user characterizations in a single ECal module. There are memory limitations; the PNA will determine if the contents of a user characterization will fit inside the module before it is performed. **Note:** This is a new feature with PNA Rev. 3.0. Previous versions of PNA will NOT recognize more than one user characterization.
- Both 2-port and 4-port ECal modules support user characterization.


How to Perform a User Characterization

SUMMARY (A [detailed procedure](#) follows.)


1. Select adapters for the module to match the connector configuration of the DUT.

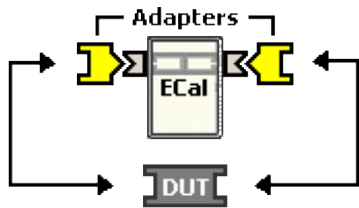


2. Either perform a Guided calibration using mechanical standards or recall a Cal Set. This is required to make accurate measurements of the ECal module and adapters.

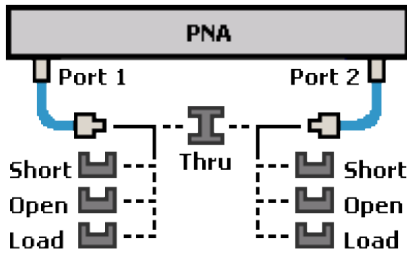

3. Measure the ECal module, including adapters, as though it were a DUT.

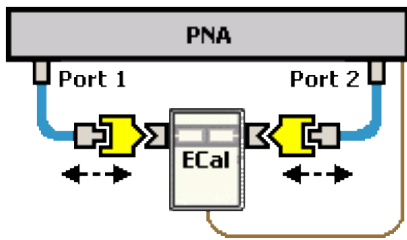

4. The measurement result is the characterization data that then gets stored inside the module.

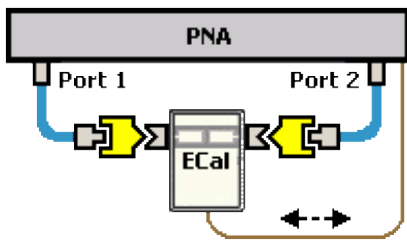

Detailed steps to Perform a User Characterization:

1. Connect the ECal module to the network analyzer with the USB cable. See [Connect ECal Module USB to PNA USB](#).
2. Allow the module to warm up until it indicates **READY**.
3. **Preset** the analyzer.
4. Set up the measurement. For best accuracy, the **IF bandwidth** should be set to **1 kHz** or less.
5. Start the **Characterize ECal Module** Wizard:

Select Connectors for the Characterization dialog box help

Note: When performing an ECal User Characterization, do NOT use a custom connector name that you added to this list. If you need to use a custom-defined connector type, modify either the "Example A" or "Example B" cal kit, which uses Type A and Type B connectors. Do NOT change the name of these connectors.

Allows you to select the adapters for the ECal module test ports. Select **No adapter** if no adapter is used on a port.


PORT A Lists the connector types available for Port A.

PORT B Lists the connector types available for Port B.

PORT C Lists the connector types available for Port C (available with a 4-port ECal module).

PORT D Lists the connector types available for Port D (available with a 4-port ECal module).

Next Click to continue to the Calibrations to perform or recall dialog box.

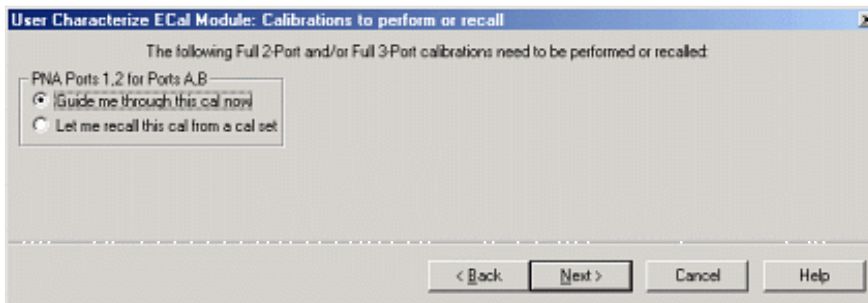


Calibrations to perform or recall dialog box help

The PNA must be calibrated before measuring the ECal module and necessary adapters. This dialog box displays the number and types of mechanical calibrations required for the characterization.

Guide me through this cal now Click to perform a Guided calibration. A calibration kit is required for each connector type.

Let me recall this cal from a cal set Click to select a Cal Set from a previous calibration for the connector types. Learn more about Using Cal Sets.

Next Click to continue to either the Select Cal Kits or the Select Cal Set dialog box.

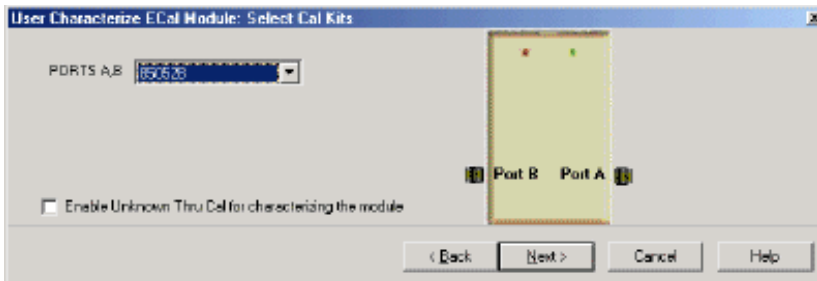


Select Cal Kits dialog box help

Provides a list of calibration kits to perform the calibration. Select the Cal Kit you will use for each port.

Enable Unknown Thru for characterizing the module Check to enable. This reduces the number of steps required to characterize the THRU standard. This setting is available only on PNA models with one reference receiver per port.

Next Click to continue to the Select Cal Set dialog box.

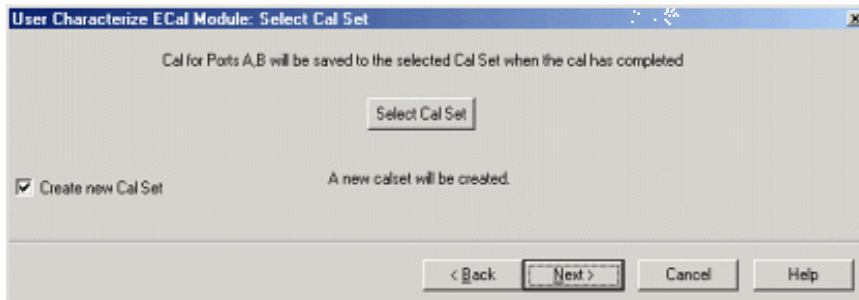

Select Cal Set dialog box help


The calibration that you perform will be written to a Cal Set. This dialog box allows you to select a Cal Set to overwrite, or to write to a new Cal Set. The current choice is visible below the **Select Cal Set** button.

Select Cal Set Click to open the **Select A Cal Set** dialog box.

Create new Cal Set Check to create a new Cal Set to store the calibration. Clear to select and overwrite a stored Cal Set.

Next Click to continue to the Guided Calibration Steps dialog box.

Note: Make a note of the Cal Set name for future reference.

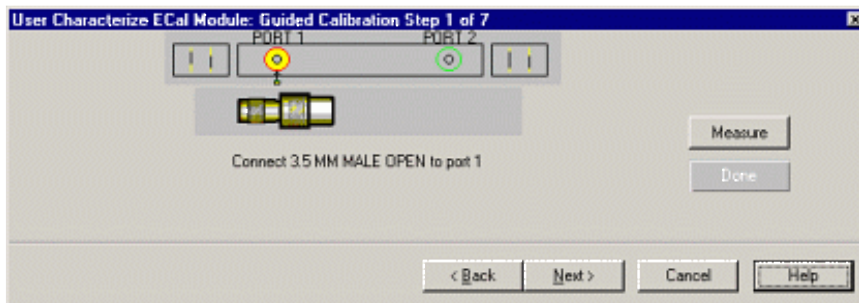

Guided Calibration Steps dialog box help

Instructs you to connect each calibration standard to the measurement port.

Measure Click to measure the standard.


Back Click to repeat one or more calibration steps.

Done Click **after** a standard is re-measured and all measurements for the calibration are complete.

Next Click to continue to the next calibration step. (Does **not** measure the standard.)

Cancel Exits Calibration Wizard.

The **Specify nominal delay** or **Guided Calibration completed** dialog box opens when the steps are completed.

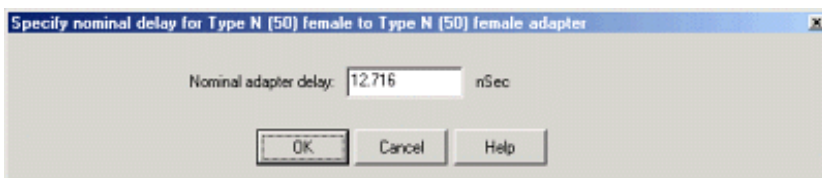

Specify nominal delay dialog box help

This dialog **ONLY** appears when Adapter Removal or Unknown THRU calibrations are performed.


An estimate of the nominal delay is required.

OK Click to accept adapter delay.

For CW sweep or frequency sweeps with large frequency steps, overwrite the estimate and then click OK.

Compute delay by calculating the physical length of the adapter divided by the propagation velocity.

Delay = Length / Propagation Velocity

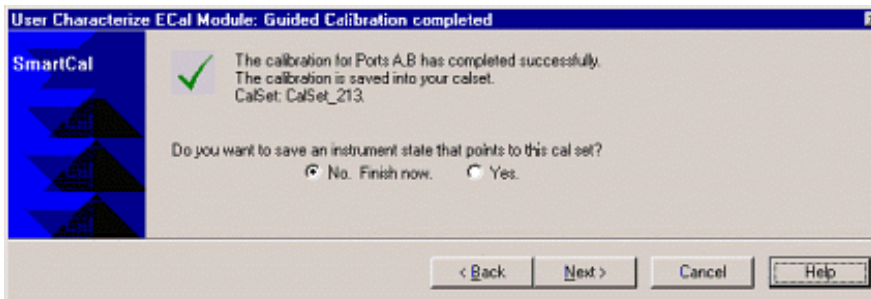


Guided Calibration completed dialog box help

Allows you to finish the calibration and continue to the next characterization steps.

No. Finish now Select to save Cal Set data.

Yes Allows selection of Save options.

Next Click to continue to the Exit to Inspect Quality of Calibration dialog box.

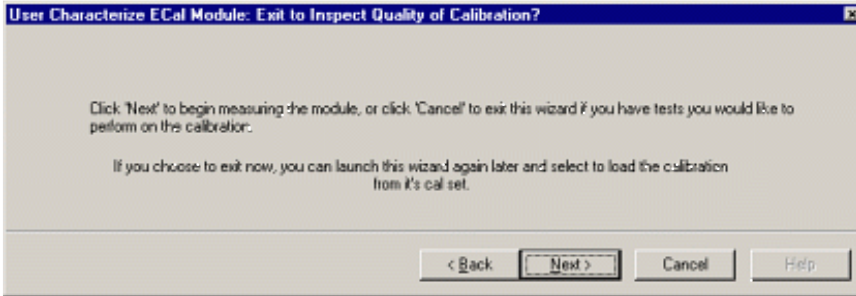

Exit to Inspect Quality of Calibration dialog box help

Allows you to exit User Characterization to validate the calibration before proceeding with the characterization.


Back Allows you to repeat calibration.

Next Click to continue to the Characterization Steps dialog box.

Cancel Exits the Calibration.

To return to the current step:

1. Start User Characterization.
2. In the **Select user number for new characterization** dialog box, click **Next**.
3. In the **Select Connectors for Characterization** dialog box, click **Next**. (Previous entry is stored in memory.)
4. In the **Calibrations to perform or recall** dialog box, recall the Cal Set that you just performed.

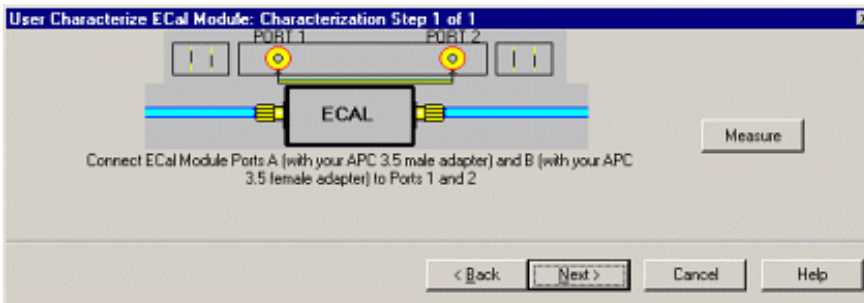

Characterization Steps dialog box help

Describes the instructions for each measurement required for characterization.

Measure Measures the ECal module.

Next Click to continue to the Information for the New Characterization dialog box when measurements are complete.

User Characterize ECal Module: Information for the New Characterization

Your name or company name:

Description of this network analyzer (to be stored in module):

Description of Port A extension (adapter, cable, fixture, etc.):

Description of Port B extension (adapter, cable, fixture, etc.):

ECal module memory limits the size of these text fields. Click 'Help' for suggestions on abbreviations for connector descriptions.

< Back Next > Cancel Help

Information for the New Characterization dialog box help


Allows you to describe the properties of the User Characterization.

Next Click to continue to the Write Characterized Data to the ECal module dialog box.

To minimize the number of characters, use the following 3-character codes to describe the connectors listed.

Connector Type	3-Character Code
1.0 mm female	10F
1.0 mm male	10M
1.85 mm female	18F
1.85 mm male	18M
2.4 mm female	24F
2.4 mm male	24M
2.92 mm female	29M
2.92 mm male	29F
3.5 mm female	35F
3.5 mm male	35M
7-16 female	16F
7-16 male	16M
Type F female	F7F
Type F male	F7M
N50 female	N5F
N50 male	N5M
N75 female	N7F
N75 male	N7M

APC 7	7MM
K-band waveguide	KBW
P-band waveguide	PBW
Q-band waveguide	QBW
R-band waveguide	RBW
U-band waveguide	UBW
V-band waveguide	VBW
W-band waveguide	WBW
X-band waveguide	XBW

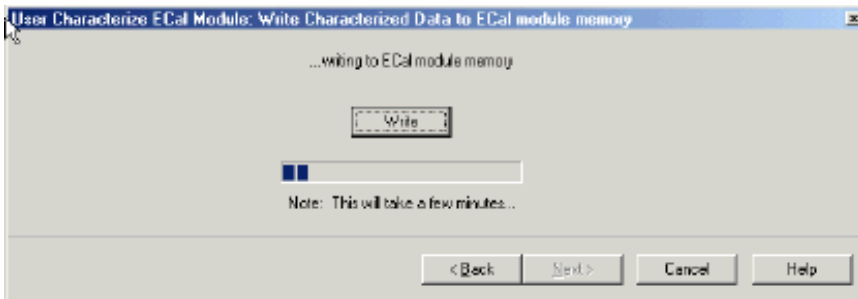


Write Characterized Data to the ECal module memory dialog box help

The PNA writes User Characterization and factory characterization data to the ECal module memory. For more information, see [Restore ECal module memory](#).

Write Click to write data into the ECal module.

The [Summary of new user characterization](#) dialog box opens after data is saved to module.

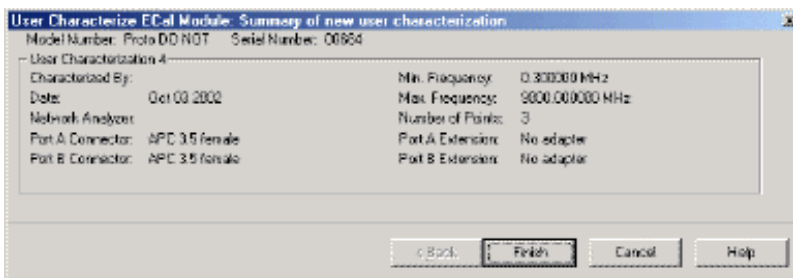

Summary of new user characterization dialog box help

Verify the status of the ECal User Characterization.

- ECal module model number
- summary from user characterization


Cancel Click to exit (characterization complete).

Finish Click to exit (characterization complete).


Restore ECal Module Memory

When user-characterized data is written to the ECal module, the entire contents of ECal memory is also written to the PNA hard drive. In the unlikely event that your ECal module memory is lost, you can restore the user-characterized data to ECal memory.

How to Restore ECal Module Memory

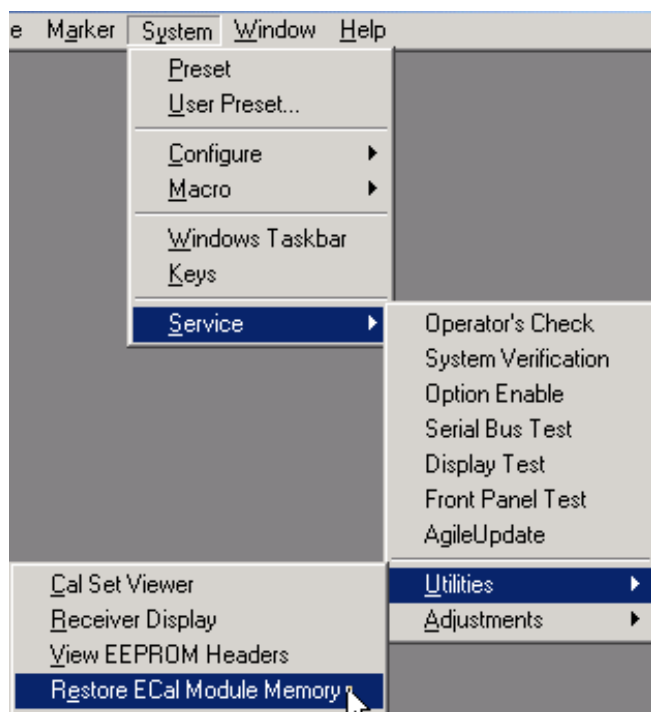

Learn more about using the [front panel interface](#)

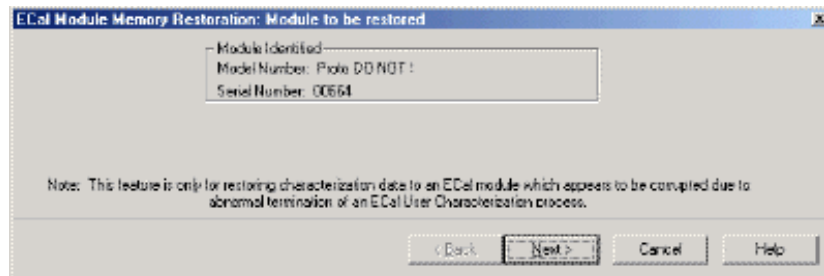

Module to be restored dialog box help

Verify the Serial number of the module to be restored. If two modules are connected to the PNA , choose the one to have data restored.

Next Click to write data to the module.

Error Correction and Interpolation

Error Correction and Interpolation settings work together to provide you with the highest level of calibration accuracy possible.

[How to set Error Correction and Interpolation](#)


[Error Correction](#)

[Viewing Correction Levels](#)

[Interpolation and Accuracy](#)

See other Calibration Topics

How to set Error Correction and Interpolation

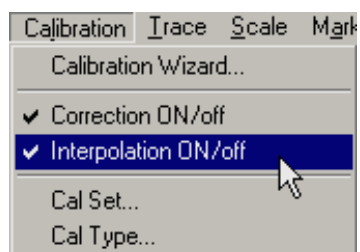

Learn more about using the [front panel interface](#).

Error Correction

The Error Correction ON setting means that the calibration error terms are applied to the measurement. Error Correction is automatically turned ON when a calibration is performed or if a Cal Set is applied to a measurement. The PNA attempts to turn error correction ON for ALL of the measurements on the active channel. This may not always be possible when applying Cal Sets. For more information, see [Applying Cal Sets](#).

You can always turn Error Correction OFF for the active measurement by clicking Correction OFF. The PNA will turn Error Correction OFF automatically when making stimulus changes under some conditions. To turn correction back ON, click **Correction ON**. Then:

- If Interpolation can NOT be performed, a dialog box will ask if you would like to change the stimulus settings to those of the applied calibration. Click OK or Cancel.
- If Interpolation can be performed, the stimulus setting will change and correction turned ON.

Interpolation

Calibration interpolation adjusts calibration error terms to match changes to the following settings that you make AFTER a calibration is performed or a Cal Set applied.

The Interpolation **ON** setting means that interpolation is **enabled** for the active measurement. This does not necessarily mean that the measurement is interpolated. When enabled (ON), if interpolation becomes necessary because you change any of the following stimulus settings, **then** interpolation will be applied. When stimulus

settings change while interpolation is OFF, interpolation is NOT applied but instead, error correction is turned OFF. Interpolation occurs (if enabled) when you change any of the following settings:

- Start frequency increased
- Stop frequency decreased
- Number of points


Note: Decreasing the start frequency, or increasing the stop frequency will always turn correction **OFF**. (Exception: Power Calibration DOES extrapolate to the start and stop frequencies.)

Viewing Correction Level

The correction level provides information about the accuracy of the active measurement. Correction level notation is displayed on the status bar for different calibration types like response, full 2-port, TRL or power calibration.

To View Correction Levels:

In the **View** menu, click **Status Bar**. The status bar appears and displays the following items:



- Active Channel
- Measurement parameter
- Correction Level (see description below)
- Calibration type

	Correction Level	Accuracy
C	Full	Highest
C*	Interpolated	Uncertain
CΔ	Changed	Uncertain
No Cor	No Correction	Lowest

C Full Correction

Full Correction level is displayed immediately after a calibration is performed or when a valid Cal Set is applied. If you require optimum accuracy, avoid adjusting analyzer settings after calibration so your measurement remains at this level.

C* Interpolated Correction

"C star" appears in the status bar when a measurement is being interpolated. See Interpolation (above) and [Interpolation Accuracy](#).

CD Changed Settings

"C-delta" appears in the status bar when one or more of the following stimulus settings change. The resulting measurement accuracy depends on which parameter has changed and how much it has changed. For optimum accuracy, recalibrate using the new settings.

- Sweep time
- IF Bandwidth
- Port power
- Stepped sweep enabled/disabled

No Corr No Correction

The following will cause the PNA to turn Error Correction OFF for the channel:

- Decrease the start frequency
- Increase the stop frequency
- Change start frequency, stop frequency, or number of points with Interpolation OFF.
- Change sweep type

Interpolation Accuracy

When a measurement is interpolated, the accuracy of the measurements cannot be predicted. It may be affected significantly or not at all. Identifying measurement errors in these cases must be determined on a case-by-case basis.

Significant measurement inaccuracy WILL occur when the phase shift between measurement points increases more than 180 degrees. The PNA will incorrectly interpolate the new phase data. For more information, see [phase accuracy](#).

In general, the chances of significant inaccuracy increases when interpolating measurements under the following conditions:

- when increasing, rather than decreasing, the frequency span between measurement points.
- when frequency span between measurement points becomes much greater.
- when measurement frequencies are very high, especially above 10 GHz.

Accurate Measurement Calibrations

Calibration accuracy is affected by the type of calibration, quality of the calibration standards, and the care with which the calibration is performed. This section provides additional information about how to make accurate calibrations.

[Measurement Reference Plane](#)

[Effects of Using Wrong Calibration Standards](#)

[Data-based versus Polynomial Calibration Kits](#)

[Accuracy Level of Interpolated Measurement](#)

[Effects of Power Level](#)

[Setting System Impedance](#)

[Using Port Extensions](#)

[Isolation Portion of 2-Port Calibration](#)

[Choosing a Thru Method](#) (separate topic)


Learn how to [determine the validity of your calibration](#).

[See other Calibration Topics](#)

Measurement Reference Plane

Most measurement setups will NOT allow you to connect a device under test directly to the analyzer's front panel test ports. More likely, you would connect your device to test fixtures or cables that are connected to the analyzer.

For the highest measurement accuracy, you should calibrate at the points where you connect your device. This is called the measurement reference plane (see graphic). If you calibrate at these points, the errors associated with the test setup (cables, test fixtures, and adapters used between the analyzer ports and the reference plane) are measured and removed in the calibration process.

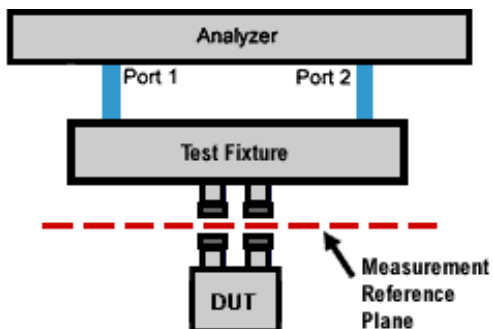

Effects of Using Wrong Calibration Standards

Normally, a calibration is performed using a calibration kit that contains standards with connectors of the same type and sex as your device under test.

However, your calibration kit may not have the same connector type as your device. For example, suppose your device has 3.5mm connectors, but you have a Type-N calibration kit. So, you use an adapter to connect the Type-N standards to the 3.5mm test port. Because the adapter is part of the calibration and NOT part of the test setup, this will result in significant errors in your reflection measurements.

Data-based versus Polynomial Calibration Kits

The [Select DUT Connectors and Cal Kits](#) dialog box offers a data-based model and a polynomial model for the newest high-frequency cal kits. See PNA Accessories. The data-based models provide higher accuracy for describing calibration standards than the polynomial models. It is RECOMMENDED that the data-based model be used if the most accurate results are desired.

	Data-Based Model	Polynomial Model
How accurate is the model?	Provides highest calibration accuracy. Eliminates the errors that can be the result of polynomial model approximations.	Provides high calibration accuracy.
How does the model define calibration standards?	Uses S-Parameter measurements.	Uses traditional four-term polynomial calibration standard modeling parameters.
How do I manually edit the definitions of the calibration standards when using the model?	Use the Advanced Modify Cal Kit function.	Use the Advanced Modify Cal Kit function.
How do I use the Calibration Wizard with the model?	Use only the SmartCal (Guided) Calibration method.	Use the SmartCal (Guided) or the Unguided Mechanical Calibration methods.

Learn about the [“Expanded Math”](#) feature.

Effects of Power Level


To attain the most accurate error correction, do NOT change the power level after a calibration is performed. However, when changing power within the same attenuator range at which the measurement calibration was performed, S-parameter measurements can be made with only a small degradation of accuracy. If a different attenuator range is selected, the accuracy of error correction is further degraded.

To check the accuracy of a calibration, see [Validity of a Calibration](#).


Setting System Impedance

The system impedance can be changed for measuring devices with an impedance other than 50 ohms, such as waveguide devices.

How to change the System Impedance

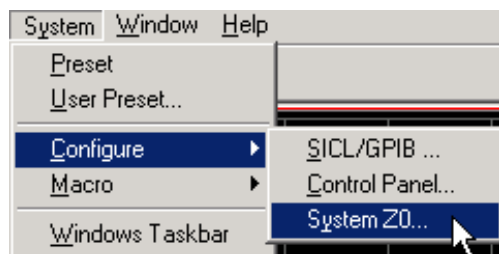

Learn more about using the [front panel interface](#)

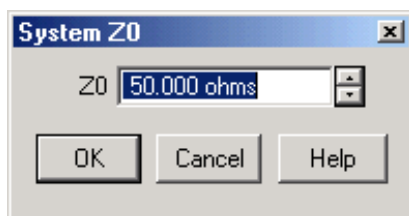

System Z0 dialog box help

Allows you to change the system impedance (default setting is 50 ohms).

Z0 Displays the current system impedance.

For 75 ohm devices:

1. Change the system Z0 to 75 ohms.
2. Connect minimum loss pads (75 ohm impedance) between the analyzer and the DUT.
3. Perform a calibration with 75 ohm calibration standards.

For waveguide devices:

1. Change the system Z0 to 1 ohm.
2. Perform a calibration with the appropriate waveguide standards.

Using Port Extensions

Use the port extensions feature after calibration to compensate for phase shift of an extended measurement reference plane due to additions such as cables, adapters, or fixtures.

Port extensions is the simplest method to compensate for phase shift between the calibration reference plane and the DUT. Applying port extensions does not, however, compensate for the mismatch and loss of the path between the reference plane and the DUT. For this reason, you should minimize the loss and mismatch caused by a test fixture to achieve best measurement accuracy.

To learn how to apply port extensions, see [Port Extensions](#).

To learn about characterizing a test fixture, see [Fixturing](#).

Isolation Portion of 2-Port Calibration

The isolation portion of a calibration corrects for crosstalk, the signal leakage between test ports when no device is present. When performing an UNGUIDED 2-port calibration, you have the option of omitting the isolation portion of the calibration.

Note: Isolation is never performed on a Smart (Guided) Calibration.

The uncorrected isolation between the test ports of the PNA is exceptional (typically >100dB). Therefore, you should only perform the Isolation portion of a 2-port calibration when you require isolation that is better than 100dB. Perform an isolation calibration when you are testing a device with high insertion loss, such as some filter stopbands or a switch in the open position.

The isolation calibration can add noise to the error model when the measurement is very close to the noise floor of the analyzer. To improve measurement accuracy, set a narrow IF Bandwidth.

How to perform an isolation calibration

Isolation is measured when the Load standards are connected to the PNA test ports. For best accuracy, connect Load standards to BOTH test ports each time you are prompted to connect a load standard. If two Loads are not available, connect to the untested PNA port any device that will present a good match.

Validity of a Calibration

This section helps you determine if your calibration is valid and how the analyzer displays correction level information for your measurement.

[Validating a Calibration](#)

[Quick Check](#)

[Cal Confidence Check](#)

[Verification Kit](#)

[See other Calibration Topics](#)

Validating a Calibration

At the completion of a calibration or selection of a stored Cal Set, validation can accomplish the following:

Improve Measurement Accuracy – Once a measurement calibration has been performed, its performance should be checked before making device measurements. There are several sources of error that can invalidate a calibration: bad cables, dirty or worn calibration standards that no longer behave like the modeled standards, and operator error.

Verify Accuracy of Interpolation – You should validate the calibration if you are testing a device and the measurements are uncertain because of interpolation. For more information see [Interpolation Accuracy](#).

Verify Accuracy of Cal Standards – To check accuracy, a device with a known magnitude and phase response should be measured.

Quick Check

For this test, all you need are a few calibration standards. The device used should not be one of the calibration standards; a measurement of one of these standards is merely a measure of repeatability. The reflection and transmission tests can be applied to all test ports.

 **verify reflection measurements, perform the following steps:**

1. Connect either an OPEN or SHORT standard to port 1. The magnitude of S11 should be close to 0 dB (within a few tenths of a dB).
2. Connect a load calibration standard to port 1. The magnitude of S11 should be less than the specified calibrated directivity of the analyzer (typically less than -30 dB).

To verify transmission measurements:

1. Connect a THRU cable (or known device representative of your measurement) from port 1 to port 2. Verify the loss characteristics are equivalent to the known performance of the cable or device.
2. To verify S21 isolation, connect two loads: one on port 1 and one on port 2. Measure the magnitude of S21 and verify that it is less than the specified isolation (typically less than -80 dB).

Note: To get a more accurate range of expected values for these measurements, consult the analyzer's

specifications.

ECal Confidence Check


ECal Confidence Check is a method to check the accuracy of a calibration performed with mechanical standards or an ECal module. The confidence check allows you to measure an impedance state in the ECal module (called the confidence state), and compare it with factory measured data stored in the module.

In order for this test to be valid, the test ports of the ECal module must connect directly to the calibration reference plane (without adapters).

Note: ECAL Confidence Check does not work with a 4-port ECAL module

To Perform ECal Confidence Check:

1. Connect ECal module to the analyzer with the USB cable. See [Connect ECal Module to the PNA](#). **Note:** Terminate any unused ECAL ports with a 50 ohm load.
2. Allow the module to warm up for 15 minutes (20 minutes for a four-port module) or until the module indicates **READY**.
3. To start ECal Confidence Check, press **Menu/Dialog**, tab to the **Calibration** menu, and then click **ECal Confidence Check**.

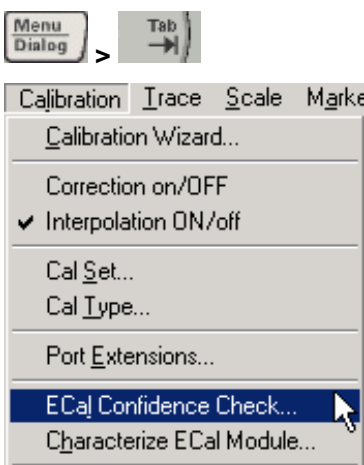

The [ECal Confidence Check dialog box](#) opens.


4. Click **Read Module Data**. The following occurs:
 - ECal module is set to "confidence state".
 - Analyzer reads and displays stored data.
 - Analyzer measures and displays "confidence state".
5. If you want to view a different parameter, select **Change Measurement** and select the check box for the desired parameter. (The default is the active channel parameter).
6. Select the viewing option in the Trace View Options block.
7. Compare the stored and measured data for each measurement parameter.

Notes:

- If the two traces show excessive difference, there may be a loose or dirty connection at the test ports or

damage to the test cables. Carefully inspect the cables and connections. Then clean and gage each connector, and re-calibrate if needed.

- The User Characterization setting selects the user-characterization data instead of the factory characterization data (available when a User-Characterization is stored in the ECal module).

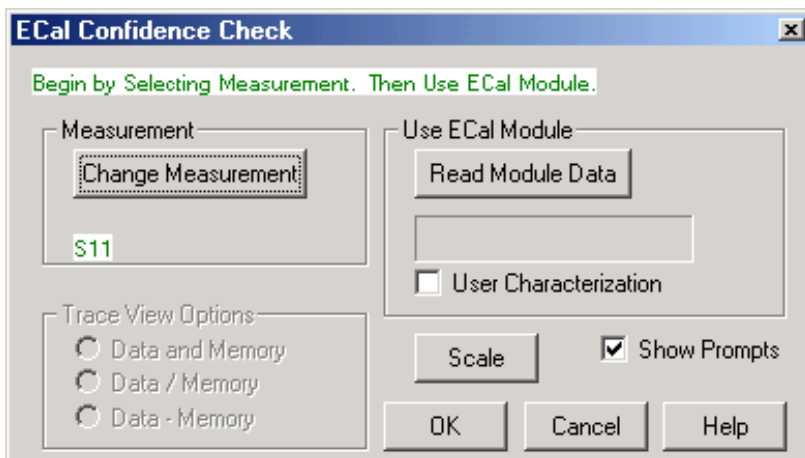

ECal Confidence Check dialog box help

Compares the accuracy of corrected (calibrated) data with stored data in the ECal module. For the check to be valid, the module test ports must connect directly to the calibration reference plane (without an adapter).

Measurement

Change Measurement Opens the Measure dialog box.

Use ECal Module

Read Module Data

- Copies stored data from the ECal module to Memory.
- Changes state of ECal module to confidence state.
- Measures and displays confidence state and Memory trace.

User Characterization Selects the user-characterization data (stored in the module) instead of the factory characterization data (available when a User-Characterization is stored in the ECal module).

Scale Opens the Scale dialog box.

Show Prompts Check to show a reminder for the connection (default).

Trace View Options

Data and Memory Trace Displays current measurement data and Memory trace.

Data / Memory Performs an operation where the current measurement data is divided by the data in memory.

Data + Memory Performs an operation where the current measurement data is added to the data in memory.

Verification Kit

Measuring known devices, other than calibration standards, is a straightforward way of verifying that the network analyzer system is operating properly. Verification kits use accurately known verification standards with well-defined magnitude and phase response. These kits include precision airlines, mismatch airlines, and precision fixed attenuators. Traceable measurement data is shipped with each kit on disk and verification kits may be re-certified by Agilent.

See [Analyzer Accessories](#) for a list of Agilent verification kits.

Measurement Errors

You can improve accuracy by knowing how errors occur and how to correct for them. This topic discusses the sources of measurement error and how to monitor error terms.

[Drift Errors](#)

[Random Errors](#)

[Systematic Errors](#)

[3-Port Error Terms](#)

[4-Port Error Terms](#)

[Monitoring Error Terms](#)

[See other Calibration Topics](#)

Drift Errors

Drift errors are due to the instrument or test-system performance changing after a calibration has been done.

Drift errors are primarily caused by thermal expansion characteristics of interconnecting cables within the test set and conversion stability of the microwave frequency converter and can be removed by re-calibrating.

The time frame over which a calibration remains accurate is dependent on the rate of drift that the test system undergoes in your test environment.

Providing a stable ambient temperature usually minimizes drift. For more information, see [Measurement Stability](#).

Random Errors

Random errors are not predictable and cannot be removed through error correction. However, there are things that can be done to minimize their impact on measurement accuracy. The following explains the three main sources of random errors.



Instrument Noise Errors

Noise is unwanted electrical disturbances generated in the components of the analyzer. These disturbances include:

- Low level noise due to the broadband [noise floor](#) of the receiver.
- High level noise or jitter of the trace data due to the noise floor and the [phase](#) noise of the LO source inside the test set.

You can reduce noise errors by doing one or more of the following:

- Increase the source power to the device being measured - ONLY reduces low-level noise.
- Narrow the IF [bandwidth](#).
- Apply several measurement sweep averages.

Switch Repeatability Errors

Mechanical RF switches are used in the analyzer to switch the source attenuator settings.

Sometimes when mechanical RF switches are activated, the contacts close differently from when they were previously activated. When this occurs, it can adversely affect the accuracy of a measurement.

You can reduce the effects of switch repeatability errors by avoiding switching attenuator settings during a critical measurement.

Connector Repeatability Errors

Connector wear causes changes in electrical performance. You can reduce connector repeatability errors by practicing good connector care methods. See [Connector Care](#).

Systematic Errors

Systematic errors are caused by imperfections in the analyzer and test setup.

- They are repeatable (and therefore predictable), and are assumed to be time invariant.
- They can be characterized during the calibration process and mathematically reduced during measurements.
- They are never completely removed. There are always some residual errors due to limitations in the calibration process. The residual (after measurement calibration) systematic errors result from:
 - imperfections in the calibration standards
 - connector interface
 - interconnecting cables
 - instrumentation

Reflection measurements generate the following three systematic errors:

Directivity

Source Match

Frequency Response Reflection Tracking

Transmission measurements generate the following three systematic errors:

Isolation

Load Match

Frequency Response Transmission Tracking

Notes about the following Systematic Error descriptions:

- The figures for the following six systematic errors show the relevant hardware configured for a forward measurement. For reverse measurements, internal switching in the analyzer makes Port 2 the source and Port 1 the receiver. 'A' becomes the transmitted receiver, 'B' becomes the reflected receiver, and 'R2' becomes the reference receiver. These six systematic errors, times two directions, results in 12 systematic errors for a two port device.
- For simplicity, it may be stated that ONE standard is used to determine each systematic error. In reality, ALL


How the Analyzer Measures and Reduces Isolation Error

1. During calibration, load standards are connected to both Port 1 and Port 2.
2. The signal measured at the 'B' receiver is leakage through various paths in the analyzer.
3. This isolation error is mathematically removed from subsequent transmission measurements.

Source Match Error

Ideally in reflection measurements, all of the signal that is reflected off of the DUT is measured at the 'A' receiver. In reality, some of the signal reflects off the DUT, and multiple internal reflections occur between the analyzer and the DUT. These reflections combine with the incident signal and are measured at the 'A' receiver, but not at the 'R' receiver.

This measurement error is called source match error which can be characterized and reduced by the analyzer.

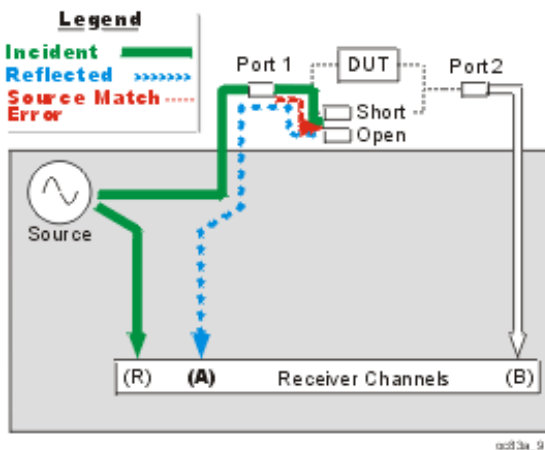

How the Analyzer Measures and Reduces Source Match Error


1. During calibration, all reflection standards are connected to Port 1. Known reflections from the standards are measured at the 'A' receiver.
2. Complex math is used to calculate source match error.
3. Source match error is mathematically removed from subsequent reflection and transmission measurements.

Load Match Error

Ideally in transmission measurements, an incident signal is transmitted through the DUT and is measured at the 'B' receiver.

In reality, some of the signal is reflected off of Port 2 and other components and is not measured at the 'B' receiver.

This measurement error is called load match error which can be characterized and reduced by the analyzer.

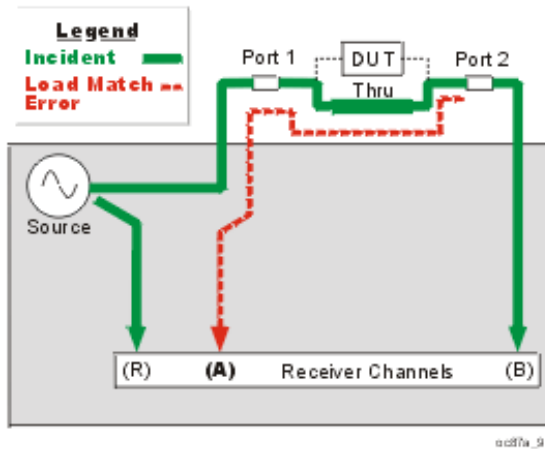

How the Analyzer Measures and Reduces Load Match Error

1. The Port 1 and Port 2 test connectors are mated together for a perfect zero-length thru connection. If this is not possible, a characterized thru adapter is inserted. This allows a known amount of incident signal at Port 2.
2. The signal measured at the 'A' receiver is reflection signal off of Port 2
3. The resulting load match error is mathematically removed from subsequent transmission and reflection measurements.

Frequency Response Reflection Tracking Error


Reflection measurements are made by comparing signal at the 'A' receiver to signal at the 'R1' receiver. This is called a ratio measurement or "A over R1" (A/R1).

For ideal reflection measurements, the frequency response of the 'A' and 'R1' receivers would be identical.

In reality, they are not, causing a frequency response reflection tracking error. This is the vector sum of all test variations in which magnitude and phase change as a function of frequency. This includes variations contributed by:


- signal-separation devices
- test cables
- adapters
- variations between the reference and test signal paths

Frequency response reflection tracking error can be characterized and reduced by the analyzer.

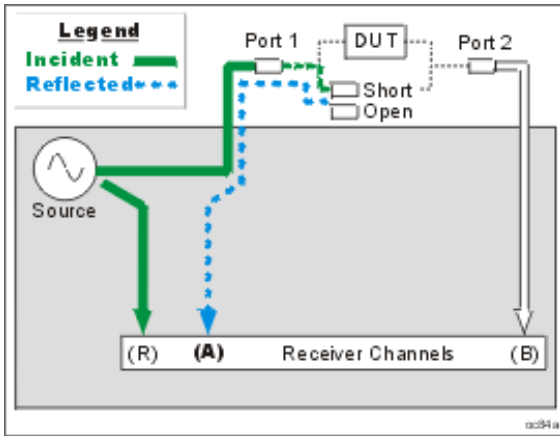

How the Analyzer Measures and Reduces Frequency Response Reflection Tracking Error.

1. During calibration, all reflection standards are used to determine reflection tracking.
2. The average 'A' receiver response is compared with the 'R1' receiver response.
3. Complex math is used to calculate Frequency Response Reflection Tracking Error (see the following diagram). This frequency response reflection tracking error is mathematically removed from subsequent DUT measurements.

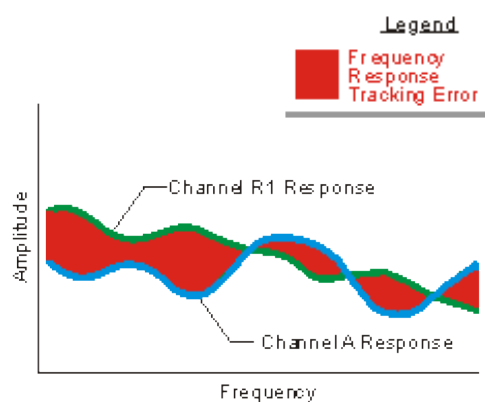

Note: In reflection response calibrations, only a single calibration standard is measured (open or short) and thus only its contribution to the error correction is used.

Frequency Response Transmission Tracking Error


Transmission measurements are made by comparing signal at the 'B' receiver to signal at the 'R1' receiver. This is called a ratio measurement or "B over R1" (B/R1).

For ideal transmission measurements, the frequency response of the 'B' and 'R1' receivers would be identical.

In reality, they are not, causing a frequency response transmission tracking error. This is the vector sum of all test variations in which magnitude and phase change as a function of frequency. This includes variations contributed by:


- signal-separation devices
- test cables
- adapters
- variations between the reference and test signal paths

Frequency response transmission tracking error can be characterized and reduced by the analyzer.

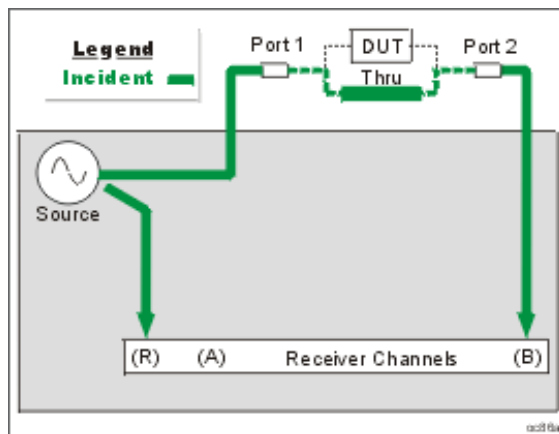


How the Analyzer Measures and Reduces Frequency Response Transmission Tracking Error.

1. During calibration, the Port 1 and Port 2 test connectors are mated together for a perfect zero-length thru connection. If this is not possible, a characterized thru adapter is inserted. This allows a known amount of incident signal to reach Port 2.
2. Measurements are made at the 'B' and 'R1' receivers.
3. Complex math is used to calculate Frequency Response Transmission Tracking Error (see the following diagram). This frequency response transmission tracking error is mathematically removed from subsequent DUT measurements.

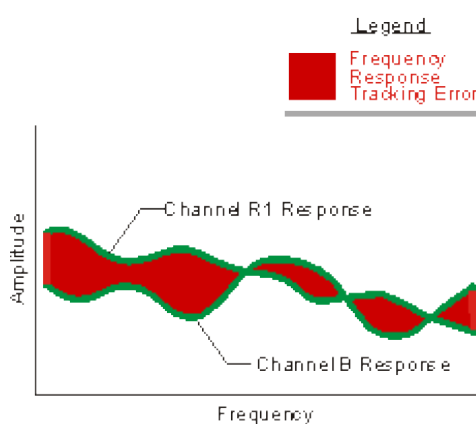

3-Port Error Terms

The following flow diagram displays the 3-port error term model:

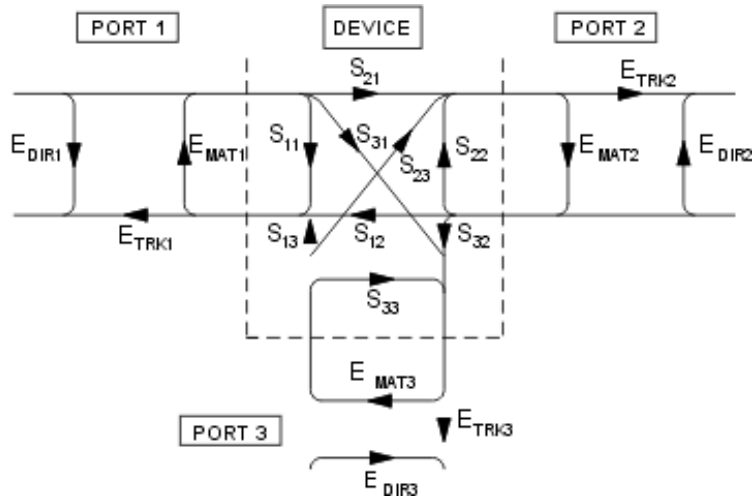

where:

E = error term

DIR = Directivity

MAT = Forward Source Match and Reverse Load Match

TRK = Forward Reflection Tracking and Reverse Transmission Tracking

4-Port error terms

A full 4-port calibration (4-port PNA model N5230 opt 240 and 245) requires the following terms:

		PORT B			
		1	2	3	4
P O R T A	1	DIR,1,1	LDM,1,2	LDM,1,3	LDM,1,4
		RTRK,1,1	TTRK,1,2	TTRK,1,3	TTRK,1,4
		SRM,1,1	XTLK,1,2	XTLK,1,3	XTLK,1,4
	2	LDM,2,1	DIR,2,2	LDM,2,3	LDM,2,4
		TTRK,2,1	RTRK,2,2	TTRK,2,3	TTRK,2,4
		XTLK,2,1	SRM,2,2	XTLK,2,3	XTLK,2,4
	3	LDM,3,1	LDM,3,2	DIR,3,3	LDM,3,4
		TTRK,3,1	TTRK,3,2	RTRK,3,3	TTRK,3,4
		XTLK,3,1	XTLK,3,2	SRM,3,3	XTLK,3,4
	4	LDM,4,1	LDM,4,2	LDM,4,3	DIR,4,4
		TTRK,4,1	TTRK,4,2	TTRK,4,3	RTRK,4,4
		XTLK,4,1	XTLK,4,2	XTLK,4,3	SRM,4,4

Reflection terms

- DIR: Directivity
- RTRK: Reflection Tracking

- SRM: Source Match

Transmission terms

- LDM: Load Match
- TTRK: Transmission Tracking
- XTLK: Cross Talk

How can we measure only 3 THRU connections?

On the 4-port PNA, a full 4-port cal can be performed while measuring only 3 THRU connections. Measuring more than 3 THRU connections will give higher accuracy.

By measuring all of the reflection terms, and 3 transmission THRU connections, there is adequate information available to calculate the remaining transmission terms. The following is a high level explanation of the concept. The actual calculations are much more complex.

To simplify, let's substitute letters (A,B,C,D) for port numbers from the diagram above so that they can be combined without confusion. Also for simplicity, let's assume that the source match and directivity errors are zero.

	A	B	C	D
A	AA	AB	AC	AD
B	BA	BB	BC	BD
C	CA	CB	CC	CD
D	DA	DB	DC	DD

- The reflection errors are all measured (AA, BB, CC, DD).
- Lets assume we measure a THRU between ports AB, AC, AD. The reverse direction for these THRU's are also measured at the same time (BA, CA, DA).
- The terms left to calculate are BC, CB, BD, DB, CD, DC.

The following shows how the BC term is calculated from BA and AC:

$$\frac{BA * AC}{AA} = \frac{B * \cancel{AA} * C}{\cancel{AA}} = BC$$

Similarly:

- CB is calculated from CA and AB
- BD is calculated from BA and AD
- DB is calculated from AB and DA
- CD is calculated from CA and AD
- DC is calculated from DA and AC

Monitoring Error Terms using Cal Set Viewer



You can use **Cal Set Viewer** to monitor the measured data and the calculated error term. This will help to determine the health of your PNA and the accuracy of your measurements.

By printing or saving the error terms, you can periodically compare current error terms with previously recorded error terms that have been generated by the same PNA, measurement setup, and calibration kit. If previously generated values are not available, refer to Typical Error Term Data in Appendix A, "Error Terms", of the Service Guide.

Note: The service guide for your PNA is available at <http://www.agilent.com/find/pna>
It is also on the CDROM that was shipped with your PNA.

- A stable system should generate repeatable error terms over about six months.
- A sudden shift in error terms over the same frequency range, power, and receiver settings, may indicate the need for troubleshooting system components. For information on troubleshooting error terms, see Appendix A , "Error Terms", of the Service Guide.
- A subtle, long-term shift in error terms often reflects drift or connector and cable wear. The cure is often as simple as cleaning and gauging connectors or inspecting cables.

How to monitor Error Terms

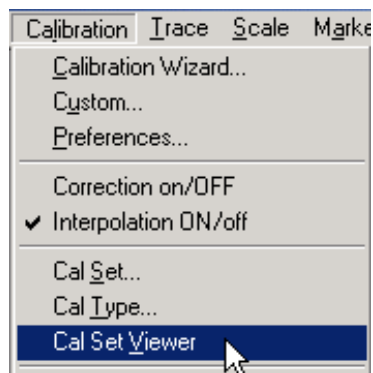

Use the down arrow to select a Cal Set

Click either

- **Error Terms** - calculated data
- **Standards** - the raw measurement data of the Standard

Use the down arrow to select the desired error term or standard of interest

Select the **Enable** check box to view the data on the PNA screen.

Learn more about using the [front panel interface](#)

Viewing Cal Set Data

- Existing measurement traces are unaffected by the Cal Set Viewer.
- The Cal Set data trace is presented in the highest unused channel number (usually 32) in the active window.

- The Cal Set data trace is labeled as S11 in the status bar regardless of the type of error term or standard.
- Only one Cal Set error term or standard data can be viewed at a time. However, you can store a data trace into memory and compare it with the same error term from another Cal Set.
- ECAL data does not include standard data, only error terms.

Automated Retrieval of Error Terms

Refer to the Data Tab of Command Finder to see the SCPI and COM commands that retrieve and store error terms.

Modify Calibration Kits

You can create or modify calibration kit files using Advanced Modify Cal Kits.

[About Modifying Calibration Kits](#)

[Creating a New Cal Kit from an Existing Cal Kit](#)

[Creating Custom Calibration Kits using a New Connector Family](#)

[How to Modify Cal Kits](#)

See other Calibration Topics

About Modifying Calibration Kits

You can modify calibration kit files or create a custom one.

Note: You CAN NOW modify Data-based Cal Kits. [Learn more.](#)

For most applications, the default calibration kit models provide sufficient accuracy for your calibration. However, several situations exist that may require you to create a custom calibration kit:

- Using a connector interface different from those used in the predefined calibration kit models.
- Using standards (or combinations of standards) that are different from the predefined calibration kits. For example, using three offset SHORTs instead of an OPEN, SHORT, and LOAD to perform a 1-port calibration.
- Improving the accuracy of the models for predefined kits. When the model describes the actual performance of the standard, the calibration is more accurate. (Example: A 7 mm LOAD is determined to be 50.40 instead of 50.00.)
- Modifying the THRU definition when performing a calibration for a non-insertable device.
- Performing a [TRL calibration](#).



Creating a New Cal Kit from an Existing Cal Kit

You can create a new custom Cal Kit using a copy of an existing Cal Kit as a starting point. Here is how:

1. From the [Edit PNA Cal Kits](#) dialog, click **Import Kit** to load the Cal Kit you want to use as a starting point. A "Duplicate Name..." message appears. Click **OK** to load a duplicate copy of the Cal kit into the last position of the Edit PNA Cal Kits dialog.
2. Select the imported kit.
3. Click **Edit Kit**, then change the [Cal Kit Name and Description](#).
4. Click **Installed Kits - Save As** to save the new Cal Kit to a .ckt file.
5. Recommended: Also click **Edit PNA Cal Kits - Save As** to save the entire collection of Cal Kits to a .wks file.
6. If using a new or modified connector, click [Change Family](#) to change the connector family.

7. Click **Add or Edit** to change connector descriptions and parameters.
8. Make modifications to your new custom Cal Kit as required. Save your work by clicking **Installed Kits - Save As**

Creating Custom Calibration Kits using a New Connector Family

To create a custom calibration kit that uses a new connector type, you must first define the connector family. The connector family is the name of the connector-type of the calibration kit, such as:

- APC7
- 2.4 mm
- Type-N (50O)

Although more than one connector family is allowed, it is best to limit each calibration kit to only one connector family.

If you are using a connector family that has male and female connectors, include definitions of both genders. If you are using a family with no gender, such as APC7, only one connector definition is required.

Use the following steps to create a custom calibration kit:

1. In the Edit PNA Cal Kits dialog box, click **Insert New** to add the new connector family.
2. In the Edit Kit dialog box:
 - Type the Kit Description for the custom cal kit.
 - Click **Add** in the Connectors section of the dialog box.
3. In the Add Connector dialog box:
 - Type a Connector Family name.
 - Type a Description of the connector.
 - Select the Gender of one of the connectors.
 - Type the minimum and maximum Frequency Range.
 - Type the Impedance.
 - Click the down-arrow to select the Media.
 - Type the cut-off frequency.
 - Click **Apply**.
 - Click **OK**.
4. If you need to add another connector gender, in the Edit Kit dialog box :
 - Click **Add** in the Connectors section again for the next connector gender.
5. If you are adding another connector gender, repeat step 3.

Note: If you have male and female versions of the connector family, you probably do NOT also have a NO GENDER version.

6. Now that the connector family is added to the custom cal kit, you are ready to add new calibration standards. In the Edit Kit dialog box:
 - Under the list of standards, click **Add**.

7. In the Add Standard dialog box:
 - Select the type of standard (OPEN, SHORT, LOAD, or THRU).
 - Click **OK**.

8. In the Edit/Add Standards dialog box:
 - Complete the information in the dialog box for the standard you selected. Note that for banded standards, the start and stop frequency may be different than the frequency range of the specified connector. Edit the start and stop frequencies as needed.
 - Click **OK** when all the settings are correct.

9. Repeat steps 6 - 8, as necessary, to add all standards and definitions to the new custom cal kit.

10. Assign each of the standards to a calibration class. This is done through the Modify Calibration Class Assignment dialog box.

11. Click **File, PrintToFile**. PrintToFile will generate a .prn file (ascii file with comma delimiters) that can be imported into a spreadsheet.


12. Import the .prn file into an application such as Microsoft Excel, and print the results.

13. Use the spreadsheet to verify that each standard in the kit belongs to the same connector family and the gender of each standard is properly specified. It is important that the connectors and genders for your standards are correctly defined and verified in order for your SmartCal (guided calibrations) to work properly.

How to Modify Cal Kits


The series of dialog boxes that follow allow you to modify the standard definitions or class assignments of calibration kit files.

How to start Advanced Modify Cal Kit

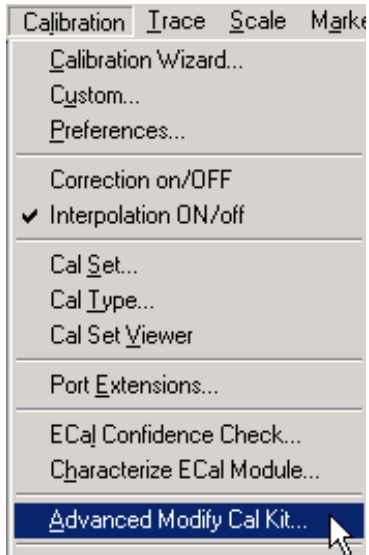

Learn more about using the [front panel interface](#)

Edit PNA Cal Kits

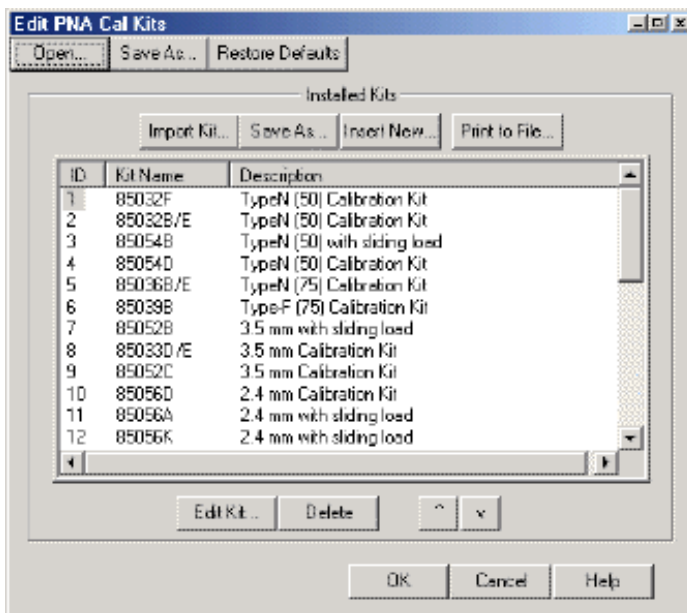

Edit PNA Cal Kits dialog box help

Provides access to all Agilent cal kits and allows modification of their standard definitions.

PNA Cal Kits and Firmware Upgrades

- The default "factory" cal kits are overwritten when new firmware is installed. Your custom cal kits (files with custom filenames) are NOT overwritten. However, the custom cal kits must be imported (click **Import Kit**) into the new firmware.
- All PNA cal kits can only be imported by the current firmware revision and later. They can NOT be imported by PAST firmware revisions. Once a Cal Kit has been imported by a later firmware revision, it cannot be imported by the previous version of firmware from which it originated.
- When a firmware upgrade takes place, ALL cal kits, both factory and custom, that are present on the PNA are saved to a single *.wks file using a unique filename. These files are NOT Excel spreadsheet files. They are opened using the **Open** button (see below). They can be used as archives of cal kits from previous firmware versions.

Open Opens an archive of cal kits from past firmware upgrades and 'Save As' operations.

Save As Saves ALL cal kits in the PNA to a *.wks file.

Restore Defaults Re-installs the default factory contents of all Agilent cal kits from the PNA hard drive. The factory Agilent cal kits are stored on the PNA hard drive at C:\Program Files\Agilent\Network Analyzer\PnaCalKits\factory.

Installed Kits

Import Kit Invokes the Import Kit dialog box.

Save As Saves the selected calibration kit and definitions (using **.ckt** file type).

Insert New Invokes a blank Edit Kit dialog box to create new calibration kit definitions.

Print to File Prints the contents of the selected cal kit to a .prn file


Edit Kit... Invokes the Edit Kit dialog box to modify selected calibration kit definitions.

Note: You CAN NOW modify Data-based Cal Kits. [Learn more.](#)

Delete Deletes selected calibration kit file.

^ Selects previous / next calibration kit in list.

For more information see [Creating Custom Calibration Kits using a New Connector Family.](#)

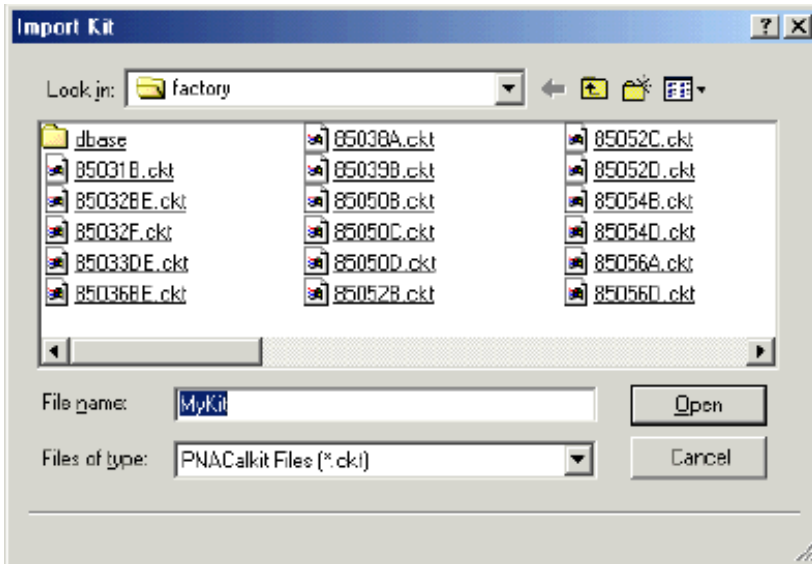

Import Kit dialog box help

Imports calibration kit definitions from hard disk or other drive that are saved in the various formats. With PNA version 4.0 or later, four kit types can be imported.

Note: See [PNA Cal Kits and Firmware Upgrades](#)

Files of type Select the file type of your Cal Kit

Cal Kit Format	File Type
Current PNA Series Cal Kit	*.ckt
Old PNA Series Cal Kit (Version 1)	*.ck1
8510 Cal Kit	CK_*
8753, 8752, 8719, 8720, or 8722 Cal Kit	*.ck


File name Navigate and select your cal kit file.

Open Imports the selected file. The kit is added at the end of the list of cal kits.

Importing Kits other than Current PNA Series Kits

Cal kit files from Agilent "legacy" network analyzers (listed above) may not contain information that the PNA requires. Therefore, the PNA may modify the cal kit name and description, the cal standards, and the cal class assignments in a "best effort" manner. You may need to correct these modifications after importing your "legacy" cal kit to meet your specific requirements.

- "Legacy" cal kit files are based on the analyzer test port sex; PNA cal kits are based on the Device Under Test (DUT) connector sex. Therefore, when the kit is imported the standard's label and description are reversed and are noted as –F- (female) and –M- (male) .
- When a Coaxial standard is detected in the kit file, a pair of male/female connectors is typically created.
- Waveguide standards that are created as "connector" have no gender.

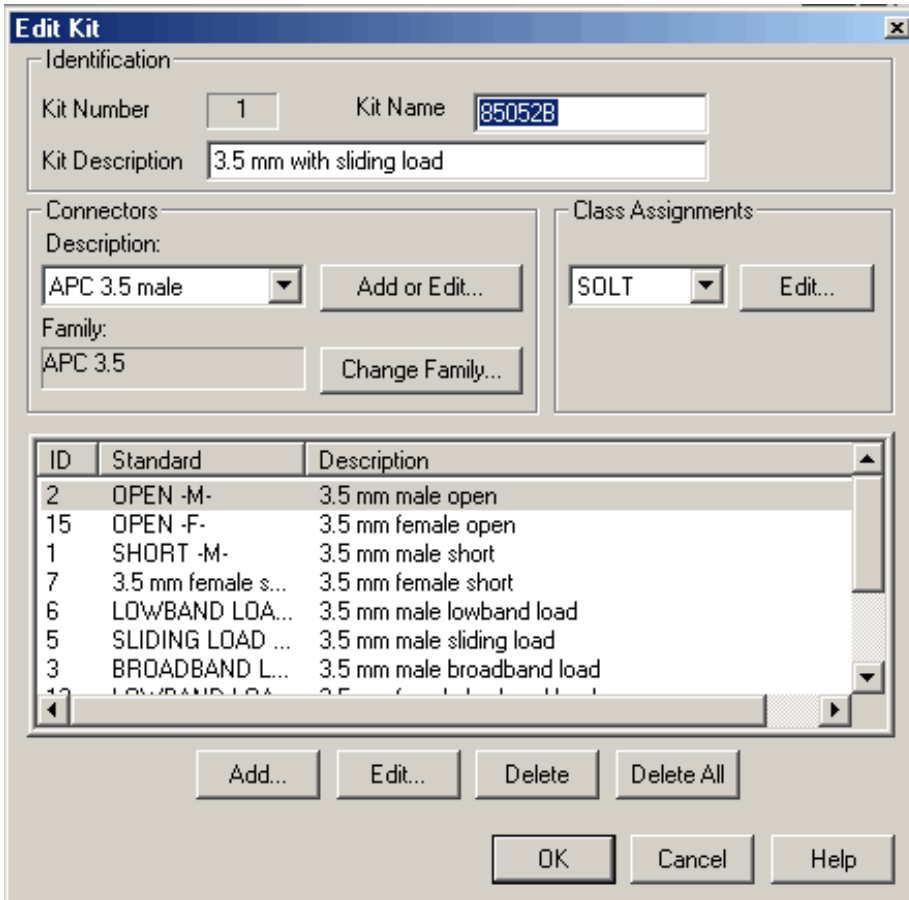

Edit Kit dialog box help

Identification

Kit Number Number of the selected calibration kit.

Kit Name Allows you to change the Name of the selected calibration kit.

Kit Description Allows you to change the description of the selected calibration kit.

Connectors

Note: You can NOT use a connector with a new or modified name to perform an ECal User Characterization.

Click the down arrow to change the connector type.

Add or Edit Invokes the Add or Edit Connector dialog box which allows you to add new connector type to the calibration kit or edit the connector properties.

Change Family Invokes the Change Connector Family dialog box which allows you to rename the entire connector family name.

Class Assignments

Click the down arrow to change the Class Assignment.

Edit Invokes the Modify Calibration Class Assignments dialog box.

Standards in Kit

Lists the current standards and descriptions in the cal kit.

Add... Invokes the Add Standard dialog box that allows you to add definitions for a standard.

Edit... Invokes the Edit dialog box that allows you to modify standard definitions for the selected standard:

either Open, Short, Load, or Thru.

Delete Deletes selected standard from calibration kit.

The screenshot shows the 'Add Connector' dialog box with the following fields and options:

- Identification:** Connector Family: Type N (50); Description: Type N (50) male
- Frequency Range:** Min: 0 MHz; Max: 999000 MHz
- Gender:** Male (selected), Female, No Gender
- Impedance:** Z0: 50 ohms
- Media:** COAX

Add or Edit Connector dialog box help

Identification

Note: You can NOT use a connector with a new or modified name to perform an ECal User Characterization.

Connector Family Allows you to Add or Edit a specific connector name. If you change Connector Family to a unique name, the name and selected Gender is ADDED to the list of connectors in that kit.

Note: To change the Connector Family Name of all connectors in the Kit, click Change Family on the previous dialog box.

Description Displays connector type and gender.

Frequency Range

Min Allows you to define the lowest frequency at which the standard is used for calibration.

Max Allows you to define the highest frequency at which the standard is used for calibration.

Gender

Allows you to define the connector gender.

Impedance


Allows you to define the impedance of the standard.

Media

Allows you to define the medium (or 'geometry') of the connector (COAX or WAVEGUIDE).

Cutoff Frequency If Media is Waveguide, type the low-end cutoff frequency.

See Also: [Creating a New Cal Kit from an existing Cal Kit](#)

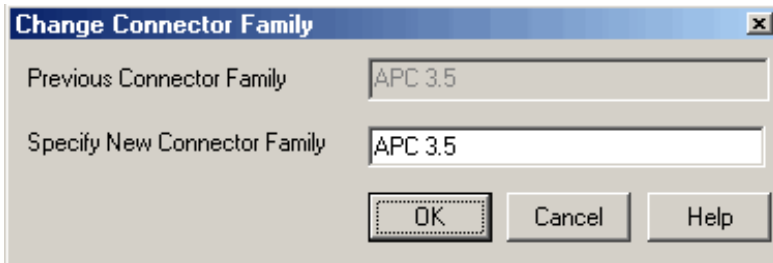

Change Connector Family dialog box help

Note: You can NOT use a connector with a new or modified name to perform an [ECal User Characterization](#).

Performs a text "Search and Replace" function. Within the description field of each of the standards of the current Cal Kit, it searches for the Previous Connector Name and replaces it with the New Connector Name.

Specify New Connector Name Allows you to replace the primary connector-family name from the selected kit with the new connector-family name. The PNA allows multiple connector-families per kit.

Previous Connector Name Displays the primary connector-family name. All occurrences of the previous connector name will be replaced throughout calibration dialog boxes. This includes calibration kit labels and description fields.

Notes:


- String replacement requires an exact match and is case sensitive. For example, "Type N" does not match "type N", and "apc 7" does not match "APC 7".
- Some calibration kits may include connector names that do not match strings within labels or description fields. You may reuse the Change Connector Name dialog to standardize the name within the kit, and then to replace the standard name with the new name.

Example:


Select the 85056A calibration kit. The default connector-family name is "APC 2.4". However, many standard description files are labeled "2.4 mm". You may want to replace the connector family name with a new name and update the standard descriptions to match the new name. For this kit, use a two step procedure.

1. Use the Change Connector Name dialog to replace "APC 2.4" with "2.4 mm".
2. Use the Change Connector Name dialog to replace "2.4 mm" with the new name, "PSC 2.4 mm".

See Also [Creating a New Cal Kit from an existing Cal Kit](#)

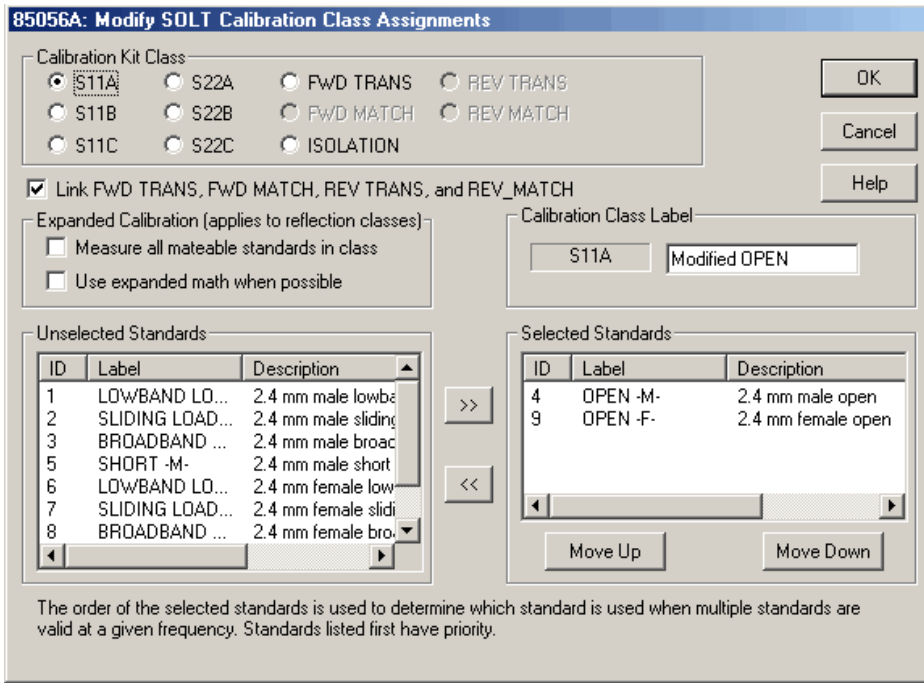

If TRL is selected as Class Assignment in the Edit Kit dialog box, the following changes appear:

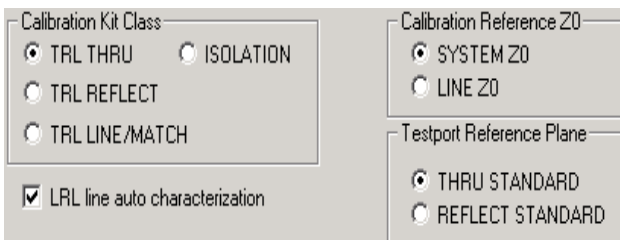

Modify Calibration Class Assignments dialog box help

Allows you to assign single or multiple standards to classes. To Add or Edit standards, click Calibration then, click [Advanced Modify Cal Kit](#).

To assign a standard to a calibration class:

1. Select the **Calibration Class**
2. Select the standard from the **Unselected Standards** field
3. Click the right arrow to move the standard to the **Selected Standards** field.


Notes:

- During an Unguided Cal all of the **Selected Standards** are presented. You then choose which of these standards to measure.
- The MATCH standards must be assigned to the FWD MATCH, REV MATCH, and LINE classes. See [TRL calibrations](#) to learn more about TRL standards.
- Use MOVE UP and MOVE DOWN to change the **ORDER** of the standard. The order is used during a [Guided Cal](#) to determine overlap priorities when:
 - **Multiple standards are valid for a frequency** - standards are presented in the order in which they appear.

- **Using two sets of standards** - modify the order in which standards appear to reflect the configuration of your DUT. For example, for a DUT with a male connector on port 1 and a female connector on port 2, order the devices within the S11 classes (A, B, and C) such that the MALE standards are first in the list. Then order the S22 classes specifying the FEMALE standards as the first in the list.

Calibration Class Label

The label that appears on the Unguided Cal - Measure Mechanical Standards dialog box. For example, the Calibration Class Label "**Modified OPEN**" would yield the following prompt:

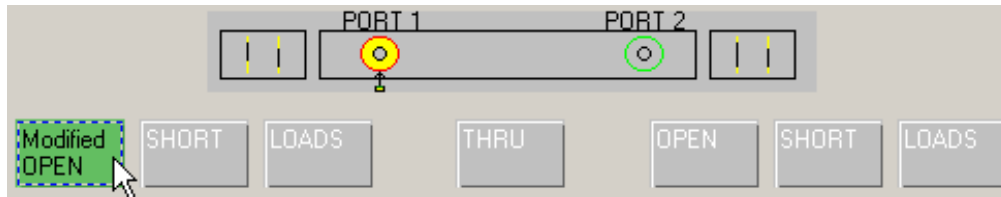

The following selections in this dialog box depend on your Class Assignment selection (**SOLT** or **TRL**) in the [Edit Kit](#) dialog box.

SOLT ONLY

Link FWD TRANS, FWD MATCH, REV TRANS, and REV MATCH Check to automatically assign the standard definition for FWD TRANS to FWD MATCH, REV MATCH, and REV TRANS. Clear to separately assign FWD MATCH, REV MATCH and REV TRANS classes (SOLT calibrations only).

Expanded Calibration

The following two check boxes **apply ONLY during Guided Calibrations**. For Unguided Calibration, these check boxes are ignored, including the case where the multiple standards dialog box is presented.

Note: You can make these selections during the calibration process with Preview/Modify settings selected from within the Cal Wizard or by modifying the cal kit from Advanced Modify Cal Kit.

Measure all mateable standards in class Check this box to attain the very highest accuracy possible. For example, if a cal kit contains several load standards, during the calibration process you will be prompted to measure each of the standards. This could require a significant amount of calibration time. When checked, the "Use expanded math when possible" box is also checked automatically.

Use expanded math when possible Some kits contain multiple calibration standards of the same type that together cover a very wide frequency range. (For example: multiple shorts, or a lowband load and a sliding load.) If a calibration requires more than one standard to cover the calibration frequency range, there can be regions of overlapping measurements. When this checkbox is selected, the PNA automatically computes the most accurate measurement in the overlap regions using a "weighted least squares fit" algorithm. This function improves accuracy without slowing the calibration speed.

- Manually select this checkbox only when using a cal kit that contains multiple standards of the same type. (For example: multiple shorts, or a lowband load and a sliding load.)
- The checkbox is cleared by default when a polynomial model is selected from the cal kit menu.
- The checkbox is selected by default when the 85058B or 85058E data-based model is selected from the cal kit menu.

TRL ONLY

The MATCH standards must be assigned to the FWD MATCH, REV MATCH, and TRL LINE classes. See [TRL calibrations](#) to learn more about TRL standards.

LRL line auto characterization

Note: This setting ONLY applies if an LRL Cal Kit is being modified **AND** Testport Reference Plane is set to Thru Standard **AND** the TRL Thru class standard and the TRL Line/Match class standard both have the same values for Offset Z0 and Loss. Otherwise, this setting is ignored.

- Check the box to allow the PNA to automatically correct for line loss and dispersion characteristics.
- Clear the box if anomalies appear during a calibrated measurement which may indicate different loss and impedance values for the Line standards.

Calibration Reference Z0 (TRL only)


System Z0 The system impedance is used as the reference impedance. Choose when the desired test port impedance differs from the impedance of the LINE standard. Also, choose when skin effect impedance correction is desired for coax lines.

Line Z0 The impedance of the line standard is used as the reference impedance, or center of the Smith Chart. Any reflection from the line standard is assumed to be part of the directivity error.

Testport Reference Plane (TRL only)

Thru Standard The THRU standard definition is used to establish the measurement reference plane. Select if the THRU standard is zero-length or very short.

Reflect Standard The REFLECT standard definition is used to establish the position of the measurement reference plane. Select if the THRU standard is not appropriate **AND** the delay of the REFLECT standard is well defined.

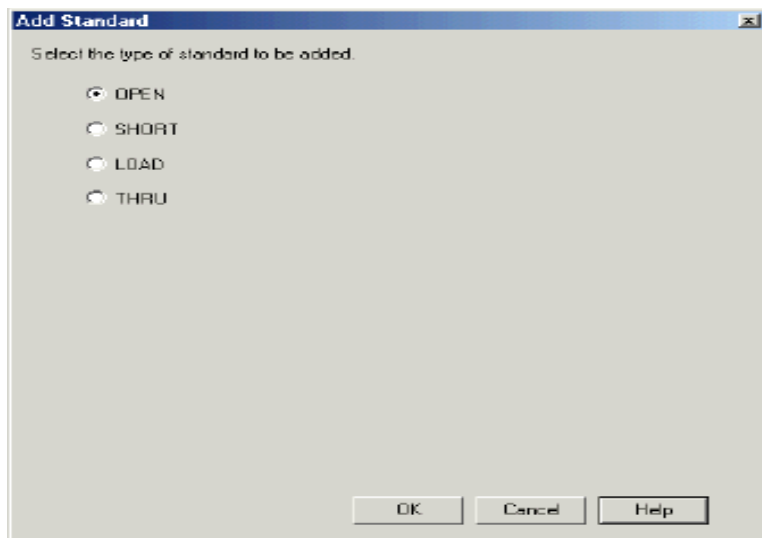

Add Standard dialog box help

Allows you to add standards to the calibration kit file.

OPEN Adds an open to the calibration kit file.

SHORT Adds a short to the calibration kit file.

LOAD Adds a load to the calibration kit file.

THRU Adds a thru to the calibration kit file.

DATA BASED STANDARD Adds a data-based standard to the calibration kit file.

OK Invokes a blank Edit Standards: Open, Short, Load, or Thru dialog box.

For more information see [Creating Custom Calibration Kits using a New Connector Family](#).

Edit / Add Standards (Open, Short, Load, Thru, or Data-based)

The screenshot shows the 'Opens' dialog box with the following fields:

- Identification:** Standard ID: 5, Label: OPEN M, Open Description: Type N (50) male open
- Frequency Range:** Min: 0 MHz, Max: 595000 MHz, Connector: Type N (50) male
- Open Characteristics:** C0: 0 F(-15), C1: 0 F(-27)Hz, C2: 0 F(-36)Hz², C3: 0 F(-45)Hz³
- Delay Characteristics:** Delay: 0 pSec, Loss: 0 Gohms/s

Edit / Add Standards dialog box help

The boxed areas of the previous graphic applies to all standard types.

The other areas change depending on the type of standard selected.

Identification

Standard ID Number in list of standards

Label Type of standard.

Description Description of standard.

Frequency Range

Min Defines the lowest frequency at which the standard is used for calibration.

Max Defines the highest frequency at which the standard is used for calibration.

Connector

Indicates the type and gender (Male, Female, None) of the standard.

Delay Characteristics

Delay Defines the one-way travel time from the calibration plane to the standard in seconds.

Z0 Defines the impedance of the standard.

Loss Defines energy loss, due to skin effect, along a one-way length of coaxial cable.

- The value of loss is entered as ohms/second at 1 GHz.
- To compute the loss of the standard, measure the delay in seconds and the loss in dB at 1 GHz. Then use the following formula:

$$\text{Loss} \left(\frac{\Omega}{\text{s}} \right) = \frac{\text{loss (dB)} \times Z_0(\Omega)}{4.3429(\text{dB}) \times \text{delay(s)}}$$

The following applies to standard types **Open**, **Short**, **Load**, **Thru**, and **Data-based**

Open Standard

Open Characteristics					
C0	<input type="text" value="89.939"/>	F(e-12)	C2	<input type="text" value="-264.9901"/>	F(e-36)/Hz^2
C1	<input type="text" value="2536.7999"/>	F(e-27)/Hz	C3	<input type="text" value="13.4"/>	F(e-45)/Hz^3

C0, C1, C2, C3 Specifies the fringing capacitance.

Short Standard

Short Characteristics					
L0	<input type="text" value="0.7563"/>	H(e-12)	L2	<input type="text" value="-52.429"/>	H(e-33)/Hz^2
L1	<input type="text" value="459.8799"/>	H(e-24)/Hz	L3	<input type="text" value="1.5846"/>	H(e-42)/Hz^3

L0, L1, L2, L3 Specifies the residual inductance.

Load Standard

Load Type	Complex Impedance
<input type="radio"/> Fixed Load	Real <input type="text" value="50"/>
<input type="radio"/> Sliding Load	Imag <input type="text" value="0"/>
<input checked="" type="radio"/> Arbitrary Impedance	

Allows you to select the type of load.

Load Type

Fixed Load Specifies the load type as Fixed

Sliding Load Specifies the load type as Sliding

Arbitrary Impedance Specifies the load type to be have an impedance value different from system Z0. Only when Arbitrary Impedance is selected are the following settings available:

- **Real** The real portion of the impedance value.

- **Imaginary** The imaginary portion of the impedance value.

Thru Standard

Connectors

Defines connector type at both ports.

Data-Based Standard

Note: To learn how to modify data-based standard files, visit <http://na.tm.agilent.com/pna/dbcal.html>

The modified file can then be uploaded into the PNA.

Upload Data From File

Click Browse to load data from a file.

Connectors

One Port Standard Currently only 1-port standards can be modified.

Port 1 Select the type of connector.

File Information Information about the standard that is read from the uploaded file.

Power Calibration

Source and Receiver Power Calibrations work together to provide very accurate power levels from the source and power measurements from the receiver.

Source Power Calibration

Reducing Time to Complete a Source Power Calibration

Receiver Power Calibration

Saving Source and Receiver Cals

See programming examples in [SCPI](#) and [COM](#)

See other Calibration Topics


Source Power Calibration

Perform Source Power Calibration when you need accurate power levels at some point in the measurement path between the PNA test ports. For example, you need to characterize the gain of an amplifier across a frequency range at a specified input power. You would perform a source power cal at the input of the amplifier to ensure the **exact** power level into the amplifier across the frequency range.

Using a Source Power Cal, you can expect the power at the point of calibration to be within the range of the uncertainty of the power meter and sensor that is used.

Note: You may not be allowed to perform a Source Power Cal unless you are logged on to the PNA with an [Administrator user account](#). To correct this, see <http://na.tm.agilent.com/pna>.

Source Power Calibration:

- Is independent of measurement type. It corrects the PNA source regardless of which receivers are being used in a measurement. Therefore, it can be used with both ratio or non-ratio measurements.
-  • Applies **ONLY** to those measurements on the selected channel that use the test port that was specified as the Source for the calibration. For example, if you specify Channel 1 and Port 1 as the source to be calibrated, only those measurements on channel 1 that use port 1 as the source will be corrected.
- Can be used in conjunction with other measurement calibrations, such as a full 2-port calibration. For highest accuracy, perform the measurement calibration **AFTER** the source calibration.
- Can be used with Power Sweep type. Source Power Cal will correct the power at all power levels across the power sweep.
- Forces sweep mode to Stepped on measurements with source power correction turned ON.

Overview of How it works:

[Click to see the detailed procedure](#)

1. Specify the measurement settings (frequency range, IFBW and so forth).

2. Start Source Power Calibration.
3. Connect a power meter sensor to the point at which you want a known power level. This may be at the input or output of your device, or some other point between the test ports.
4. The program steps the PNA source through the specified frequency range, at the specified power level, and measures the power using a power meter.
5. The program calculates and stores the difference between the desired corrected power (Cal power) and what was measured by the power meter, at each data point.
6. When complete, the power meter is preset. The source power calibration can be saved to disk as part of the instrument state.
 - The power meter is removed and the measurement path reconnected.
 - The calibration is automatically applied to the measurement so that during subsequent sweeps, the source power is adjusted by the difference values to provide the corrected power level.

Verify the source power calibration using the following procedure.

1. Connect the power meter as it was during the source power calibration.
2. Set the PNA to Point Trigger mode.
3. Trigger the PNA across the trace. Read about the behavior of the sweep indicator.
4. At each data point, the power meter should read the corrected power level within the specified tolerance.

Test Equipment Supported

Power Meters

Agilent Model Number	Critical Specification
E4416A	Single Channel
E4417A	Dual Channel
EPM-441A, E4418A/B	Single Channel
EPM442A, E4419A/B	Dual Channel
437B	Single Channel
438A	Dual Channel

See Create a Custom Power Meter Driver.


Power Sensors

You can perform a Source Power Calibration with ALL power sensors that are supported by the above list of power meters. However, Source Power Calibration and Scalar Mixer Calibration, operates slowly with the Agilent E930x and E932x power sensors, as the two calibrations are not optimized for use with those sensors.

You can use up to two sensors to cover the frequency span of the measurement.


Detailed Procedure: How to perform Source Power Calibration

1. Setup your measurement (sweep type, frequency range, IFBW, and so forth).
2. Connect coax cable, GPIB cable, and power sensors to the PNA as shown in graphic below.

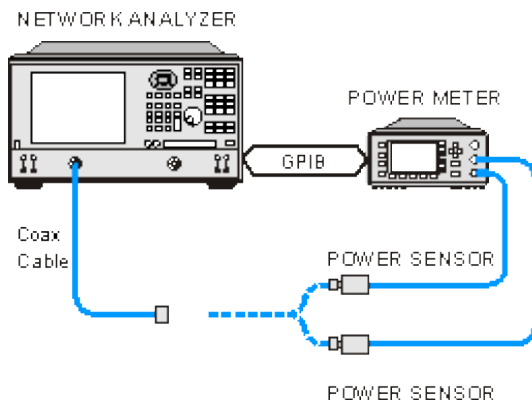

Note: You can use the [82357A USB/GPIB Interface](#) to control the power meter.

3. Apply power to the power meter and allow 30 minutes warm-up time before beginning calibration.
4. Select **Source Power Cal** as follows:

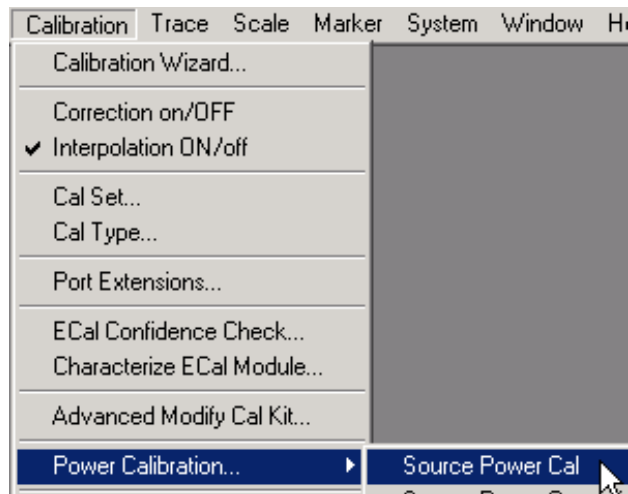


5. Complete the Source Power Cal dialog box (below), including Loss Compensation and Power Sensor Settings, as needed.
6. When complete, click **Take a Cal Sweep** in the Source Power Cal dialog box.
7. Follow the prompts to connect the sensors as required.
8. When calibration is finished, click **OK**.
9. Remove sensor.

- **SrcPwrCal** is displayed in the status bar and correction data is applied to subsequent sweeps.
- To turn correction **OFF**, on the **Calibration** menu, point to **Power Calibration**, then set **Source Power Correction** to **OFF**.

Interpolation

If the original stimulus settings are changed, Interpolation or EXTRAPOLATION is applied and **SrcPwrCal*** is displayed in the status bar. This is different from measurement calibration interpolation. For example, if the frequency span is increased, the PNA will extrapolate new correction values rather than turn correction off. This is to protect your test device from being overpowered by the source. If the original settings are restored, then source power calibration returns to full correction.

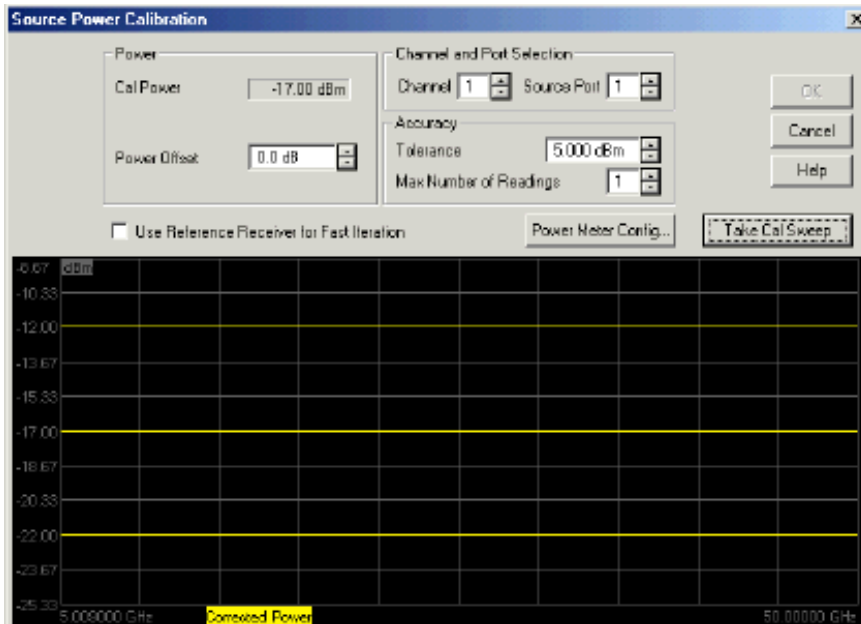

Source Power Cal dialog box help

Note: Be sure that the frequency range of your power sensor covers the frequency range of your measurement. This does NOT occur automatically.

Power

Cal Power The calculated power (in dBm) at the calibration point. This value is the specified PNA source power plus the Power Offset value.

Power Offset Allows you to specify a gain or loss (in dB) to account for components you connect between the source and the reference plane of your measurement. For example, specify 10 dB to account for a 10 dB amplifier in the path to your DUT. Following the calibration, the PNA power readouts are adjusted to this value.

Channel and Port Selection

Channel Specifies the channel on which to perform the calibration. This setting defaults to the active channel.

Source Port Specifies the selected source port. This setting defaults to the source port for the active channel.

Accuracy

At each data point, power is measured using the specified Power Meter **Settling** Tolerance and adjusted, until the reading is within this Accuracy **Tolerance** or the **Max Number of Readings** has been met. The **last** power reading is plotted on the screen against the Tolerance limit lines.

Tolerance Sets the maximum desired deviation from the specified **Cal Power** level.

Max Number of Readings Sets the maximum number of readings to take at each data point for iterating the source power.

Use Reference Receiver for Fast Iteration When checked, the first reading at each data point is used to calibrate the reference receiver. Subsequent readings, if necessary to meet your accuracy requirement, are measured using the reference receiver. This technique is much faster than using the power meter with almost no degradation in accuracy.

NOTE: Do NOT use the Reference Receiver for Iteration feature if there is a component before the power sensor that exhibits non-linear behavior, such as a power amplifier in compression.


Power Meter Config Invokes the Power Meter Settings dialog box

Take Cal Sweep Begins source power calibration measurement.

OK Applies calibration. This button is disabled until the **Take Cal Sweep** has been pressed.

Cancel Cancels calibration.

Learn more about [Source Power Cal](#)

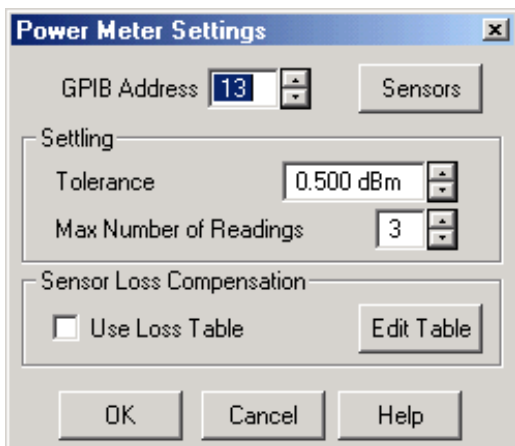

Power Meter Settings dialog box help

GPIB Address GPIB address for the power meter . Default is 13. When performing a source power cal, the PNA will search VISA interfaces that are configured in the Agilent IO Libraries on the PNA.

Sensors Invokes the [power sensor settings](#) dialog box.

Settling

Each power reading is "settled" when either:

- consecutive meter readings are within this **Tolerance** value or
- when the **Max Number of Readings** has been met.

The readings that were taken are averaged together to become the "settled" reading. The settled reading is then compared to the [Accuracy Tolerance requirements](#) (tolerance and max readings) specified on the Source Power Cal dialog box.


Tolerance When consecutive power meter readings are within this value of each other, then the reading is considered settled.

Max Number of Readings Sets the maximum number of readings the power meter will take to achieve settling.

Sensor Loss Compensation

Use Loss Table Select this checkbox to apply loss data to Source Power calibration correction (such as for an adapter on the power sensor).

Edit Table Invokes the [Power Loss Compensation](#) dialog box.

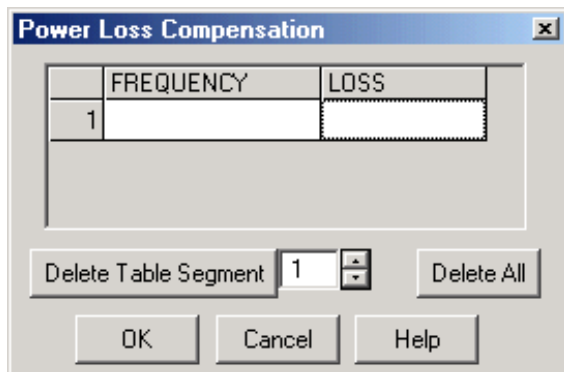

Power Loss Compensation dialog box help


Allows you to compensate for losses that occur when you use an adapter or coupler to connect the power sensor to the measurement port.

Delete Table Segment Deletes row indicated in the field.

Delete All Deletes all data in the table.

Note: To Add a Row to the table, click on a row in the table and press the down arrow on either the PNA front panel or keyboard.

- If you enter a single frequency/loss segment, the analyzer applies that value to the entire frequency range.
- You can enter up to 100 segments to achieve greater accuracy.

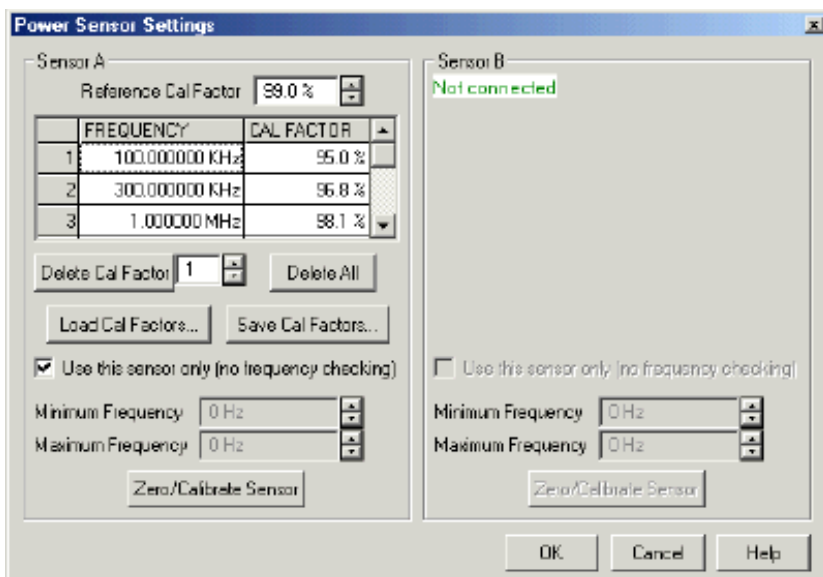

Power Sensor dialog box help

Note: Be sure that the frequency range of your power sensor covers the frequency range of your measurement. This does NOT occur automatically.

Sensor A (B) Displays one of the following messages depending on type of sensor.

- **Not connected** The PNA is not detecting a power sensor.
- **Cal factors are contained within this sensor** The PNA detects an Agilent E-Series power sensor. Reference Cal Factor and Cal Factor data are loaded automatically.
- **Sensor Data** Allows entry for power sensor data:

Reference Cal Factor Specifies the sensor's Reference Cal Factor.

Cal Factor Table Specifies the frequency and corresponding Cal Factor for the sensor.

Delete Cal Factor Deletes the indicated row in the table.

Delete All Deletes all data in the table.

Use this sensor only Select this checkbox to use this sensor over the entire frequency span of the measurement, even if two sensors are connected to power meter. Clear to allow entry of minimum and maximum frequencies for the sensor.

Minimum Frequency Specifies the minimum frequency range for the sensor when using dual sensors.

Maximum Frequency Specifies the maximum frequency range for the sensor when using dual sensors.

Perform Sensor Zeroing and Calibration Zero and calibrate the power sensor before taking data.

Note: To Add a Row to the table, click on a row in the table and press the down arrow on either the PNA front panel or keyboard. A row is added to the bottom of the table. The table is automatically sorted by frequency when OK is pressed.

Reducing Time to Complete a Source Power Calibration

The time required to perform a Source Power Calibration depends on source power, number of points, and number of readings taken. You can reduce this measurement time with the following methods:

- **Reduce number of points before calibration.** You can reduce the number of points before the measurement, then return the number of points to its original value after calibration is complete and correction is ON. The analyzer will perform a linear interpolation, although with some loss in accuracy.
- **Use an Agilent E-Series sensor.** You can obtain 40+ readings per second over GPIB with this type of sensor on the PNA.
- **Increase power to the sensor.** Lower power may have longer settling time with some sensors.
- **Check Use Reference Receiver for Iteration.**

Receiver Power Calibration

Receiver power calibration mathematically removes frequency response errors in the specified PNA receiver, and adjusts readings to the same, or a value offset from, the source power calibration level. It is the same as doing **Data / Memory**, but with the data shifted to the Cal Power value.

Use Receiver Power Calibration to make very accurate absolute power (amplitude) measurements.


Receiver Power Calibration:

- Expects that a source power calibration was performed first.
- Is ONLY allowed when making absolute power (unratioed) measurements.
- Applies to all unratioed measurements in the active channel using that receiver.
- Is saved in a Cal Set.


How to perform a Receiver Power Calibration

1. Perform a Source Power Calibration.
2. Set the active measurement to unratioed. Learn How.
3. Connect a THRU line from the source port to the receiver port. If you are performing a receiver power cal on a reference receiver, no connection is necessary as the receiver is internally connected to the source.

- Ensure correction for Source Power Calibration is ON as indicated by **Src Pwr Cal** or **Src Pwr Cal*** in the status bar.
- Start the Calibration Wizard

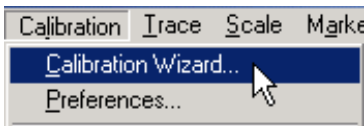

- Complete the following dialog box, then click **Next**.

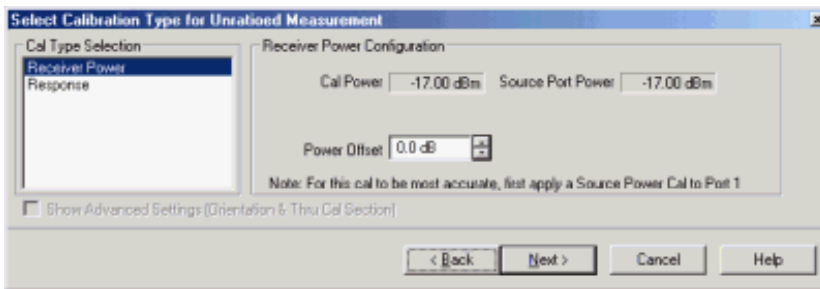

Select Calibration Type for Unratioed Measurement dialog box help

Cal Type Selection Select **Receiver Power**

Receiver Power Configuration

Cal Power Specifies the power level to be displayed on the measurement when complete. (Source Port Power + Power Offset).

Source Port Power Test port Power set for the measurement. [Learn to change Test Port Power](#)

Power Offset Allows you to specify a gain or loss (in dB) to account for components you connect between the source and the reference plane of your measurement AFTER a source power cal has been performed. Following the calibration, the PNA power readouts are adjusted to the Cal Power value.

Next Click to continue with the Calibration Wizard steps: [Take Measurement](#) and [Save Calibration](#).

Notes:

- When Receiver Power Cal is finished, **C RcvrPwr** is displayed in the status bar and correction data is applied to subsequent sweeps.
- To turn correction **OFF**, click **Calibration**, point to **Power Calibration**, then set **Receiver Power Correction** to **OFF**.

Interpolation

Like other calibration types, if the original stimulus settings are narrowed, interpolation is applied and **C* Rcvr Pwr** is displayed in the status bar. If the original stimulus settings are made wider, the PNA will turn Receiver Power Correction **OFF**.

If the original settings are restored, then receiver power calibration returns to full correction.

Saving Source and Receiver Power Calibration

A Source Power Cal is saved as part of the **Instrument State** with either a .sta file, or a .cst file. See [Save Instrument State](#).

Receiver Power Cal is saved to a [Cal Register](#) and optionally to a user [Cal Set](#).

[Learn more about Saving PNA files types.](#)

Calibration Standards

This following section explains the general principles and terms regarding calibration kit files. To learn **how** to modify calibration kit files, See [Modify Calibration Kits](#).

[About Calibration Kits](#)

[Calibration Standards](#)

[Standard Type](#)

[Standard Definitions](#)

[Class Assignments](#)

[See other Calibration Topics](#)

About Calibration Kits

A calibration kit is a set of physical devices called standards. Each standard has a precisely known or predictable magnitude and phase response as a function of frequency.


In order for the analyzer to use the standards of a calibration kit, the response of each standard must be mathematically defined and then organized into standard classes that correspond to the error models used by the analyzer.

To be able to use a particular calibration kit, the known characteristics from each standard in the kit must be entered into analyzer memory or recalled from a default list of calibration kits stored in the analyzer.

For a list of calibration kits, see [Analyzer Accessories](#).

Calibration Standards

Calibration standards provide the reference for error-corrected measurements in the network analyzer. Each standard has a precisely known definition that includes electrical delay, impedance, and loss. The analyzer stores these definitions and uses them to calculate error correction terms.

 During measurement calibration, the analyzer measures standards and mathematically compares the results with "ideal models" of those standards. The differences are separated into error terms that are later removed from device measurements during error correction.

Standard Type

A standard type is one of four basic types that define the form or structure of the model to be used with that standard. The four standard types are shown below:

Standard	Terminal Impedance
SHORT	zero ohms
OPEN	infinite ohms
LOAD	system impedance, Z0
THRU/LINE	no terminal impedance
ARBITRARY	user-defined

Standard Definitions

Standard definitions describe the electrical characteristics of the standards and the frequencies they will be used. Refer to the "standards definition table" included with the calibration kit. Standard definitions include:

- **Minimum Frequency** Specifies the minimum frequency the standard is used for calibration.
- **Maximum Frequency** Specifies the maximum frequency the standard is used for calibration.
- **Z0** Specifies the characteristic impedance of the standard (not the system characteristic impedance or the terminal impedance of the standard).
- **Delay** Specifies a uniform length of transmission line between the standard being defined and the actual calibration plane.
- **Type** Specifies type of standard (SHORT, OPEN, THRU/LINE, LOAD, ARBITRARY).
- **Loss** Specifies energy loss, due to skin effect, along a one-way length of coaxial cable.

Loss model equation:

- The value of loss is entered as ohms/second at 1 GHz.
- To compute the loss of the standard, measure the delay in seconds and the loss in dB at 1 GHz. Then use the following formula:

$$\text{Loss} \left(\frac{\Omega}{\text{s}} \right) = \frac{\text{loss (dB)} \times Z_0(\Omega)}{4.3429(\text{dB}) \times \text{delay(s)}}$$

Capacitance model equation:

C0, C1, C2, C3. Specifies the fringing capacitance for the open standard.

- $C = (C0) + (C1 \times F) + (C2 \times F^2) + (C3 \times F^3)$
- (F is the measurement frequency).
- The terms in the equation are defined when specifying the open as follows:
 - C0 term is the constant term of the third-order polynomial and is expressed in Farads.
 - C1 term is expressed in F/Hz (Farads/Hz).
 - C2 term is expressed in F/Hz².

- C3 term is expressed in F/Hz³.

Inductance model equation:

L0, L1, L2, L3. Specifies the residual inductance for the short standard.

- $L = (L0) + (L1 \times F) + (L2 \times F^2) + (L3 \times F^3)$
- (F is the measurement frequency).
- The terms in the equation are defined when specifying the short as follows:
 - L0 term is the constant term of the third-order polynomial and is expressed in Henries.
 - L1 term is expressed in H/Hz (Henries/Hz)
 - L2 term is expressed in H/Hz².
 - L3 term is expressed in H/Hz³.

Class Assignments

Once a standard is characterized, it must be assigned to a standard "class". A standard class is a group of standards that are organized according to the calibration of the PNA error model.

The number of classes needed for a particular calibration type is equal to the number of error terms being corrected.

A class often consists of a single standard, but may be composed of multiple standards, such as loads or delay lines. Refer to the calibration kit "class assignment" table.

Example: A response calibration requires only one class, and the standards for that class may include an OPEN, or SHORT, or THRU. A 1-port calibration requires three classes. A full 2-port requires 10 classes, not including two for isolation.

The number of standards assigned to a given class may vary from one to seven for unguided calibrations. Guided calibrations allow as many standards as needed.

The different classes used in the PNA:

S11A, S11B, S11C (S22A, S22B, S22C and so forth)

These are the three classes for port 1-reflection calibrations (three classes also for S22 and S33). They are used in the one-port calibrations and the full two-port calibration. They are required in removing the directivity, source match, and reflection tracking errors. Typically, these classes might consist of an open, a short and a load standard for each port.

Transmission and Match (forward and reverse)

These classes are used to perform a full two-port calibration. The transmission class relates primarily to the transmission tracking, while the match class refers to load match. For both of these classes, the typical standard is a thru or delay.

Isolation

The isolation classes are used to perform a full two-port and the TRL two-port calibrations. The isolation classes apply to the forward and reverse crosstalk terms in the PNA error model.

TRL thru

These are used to perform a TRL two-port calibration. The TRL thru class should contain a thru standard or a short line. If it contains a non-zero length thru standard, then the calibration type is called LRL or LRM.

TRL reflect

This class is used to perform a TRL two-port calibration. The TRL reflect class should contain a standard with a high reflection coefficient, typically an open or short. The actual reflection coefficient need not be known, but its

phase angle should be specified approximately correctly (± 90 deg). The exact same reflection standard must be used on both ports in the TRL calibration process.

TRL line (or match)

These are used to perform a TRL two-port calibration. The TRL line or match class should contain line standards, load standards, or both. If a line standard is used, its phase shift must differ from that of the TRL thru standard by 20° to 160° . This limits the useable frequency range to about 8 to 1. Two or more line standards of different lengths may be specified to get broader frequency coverage. It is also common to include a load standard for covering low frequencies, where the line's length would be impractically long. When a load is used, the calibration type is called TRM or LRM.

Note: For more information, read application note 8510-5A, "*Specifying Calibration Standards for the Agilent 8510 Network Analyzer*". Although the application note is written for the Agilent 8510 series of network analyzers, it applies to the PNA as well. The part number for the publication is 5956-4352.

TRL Calibration

TRL (Thru - Reflect - Line) represents a **family** of calibration techniques that measure two transmission standards and one reflection standard to determine the 2-port 12-term error coefficients. For example, TRM (Thru - Reflect - Match) is included in this family. The traditional SOLT calibration measures one transmission standard (T) and three reflection standards (SOL) to determine the same error coefficients.

[Why Perform a TRL Cal?](#)

[The TRL Calibration Process](#)

[TRL Cal Kits](#)

[Cal Standards Used in TRL](#)

[TRL Options](#)

[TRL in 4-port PNA](#)

See other Calibration Topics

Why Perform a TRL Cal?

TRL calibration is extremely accurate, in some cases more accurate than an SOLT cal. However, very few calibration kits contain TRL standards. TRL Cal is most often performed when you require a high level of accuracy and do not have calibration standards in the same connector type as your DUT. This is usually the case when using test fixtures, or making on-wafer measurements with probes. Therefore, in some cases you must construct and characterize standards in the same media type as your DUT configuration. It is easier to manufacture and characterize three TRL standards than the four SOLT standards.

A limitation for TRL cal with broad frequency coverage is the requirement for multiple LINE standards. For example, a span from 2 GHz to 26 GHz requires two line standards. Also, for lower frequencies, the LINE standard can be too long for practical use.

The TRL Cal Process

Although TRL can be performed using the Cal Wizard Unguided Cal selection, the following process uses the easier SmartCal selection. Both selections require that you already have TRL calibration standards defined and included in a PNA cal kit.

1. Preset the PNA
2. Connect the DUT to the PNA
3. Set up a S-parameter measurement and the desired stimulus settings.
4. Click **Calibration / Calibration Wizard**
5. Click **SmartCal Guided Cal / Use Mechanical Stds**
6. Select the DUT connectors and Cal Kit for each port. The **LOWEST** port number of each port pair **MUST** include TRL standards. TRL appears as the Cal Method.
7. Check **Modify Cal, Next**, then **View/Modify** to change default TRL options if necessary.

8. Follow the prompts to complete the calibration.
9. Check the accuracy of the calibration

TRL Cal Kits

Agilent Technologies offers two cal kits that include the required standards to perform a TRL calibration: 85050C (APC 7mm) and 85052C (3.5mm). Both kits include the traditional Short, Open, and Load standards. (The Thru standard, not actually supplied, assumes a zero-length Thru). In addition, the kits include an airline which is used as the LINE standard. To use the airline, the kits include an airline body, center conductor, and insertion / extraction tools. The APC 7 kit includes an adapter to connect the airline to the APC connector.

Cal Standards Used in TRL

These standards must be defined in your TRL cal kit:

THRU

Note: All THRU calibration methods are supported in a TRL Cal **EXCEPT** Unknown Thru.

- The THRU standard can be either a zero-length or non-zero length. However, a zero-length THRU is more accurate because it has zero loss and no characteristic impedance.
- The THRU standard cannot be the same electrical length as the LINE standard.
- If the insertion phase and electrical length are well-defined, the THRU standard may be used to set the reference plane.

REFLECT

- The REFLECT standard can be anything with a high reflection, as long as it is the same when connected to both PNA ports.
- The actual magnitude of the reflection need not be known.
- The phase of the reflection standard must be known within 1/4 wavelength.
- If the magnitude and phase of the reflection standard are well-defined, the standard may be used to set the reference plane.

LINE

The LINE standard establishes the reference impedance for the measurement after the calibration is completed. TRL calibration is limited by the following restrictions of the LINE standard:

- Must be of the same impedance as the THRU standard
- The electrical length need only be specified within 1/4 wavelength.
- Cannot be the same length as the THRU standard.
- Must be an appropriate electrical length for the frequency range: at each frequency, the phase difference between the THRU and the LINE should be greater than 20 degrees and less than 160 degrees. This means in practice that a single LINE standard is only usable over an 8:1 frequency range (Frequency Span / Start Frequency). Therefore, for broad frequency coverage, multiple lines are required.

- At low frequencies, the LINE standard can become too long for practical use. The optimal length of the LINE standard is 1/4 wavelength at the geometric mean of the frequency span (square root of $f_1 \times f_2$).

MATCH

If the LINE standard of appropriate length or loss cannot be fabricated, a MATCH standard may be used instead of the LINE.

- The MATCH standard is a low-reflection termination connected to both Port 1 and Port 2.
- In the TRL computation, this standard is treated as a high-loss, infinite length transmission line.
- The impedance of the MATCH standard becomes the reference impedance for the measurement.


Note: The MATCH standards must be assigned to the FWD MATCH, REV MATCH, and TRL LINE classes. See [Modify Calibration Kits](#) for detailed information about creating and modifying Calibration kit definitions.

Find more information about TRL standards at <http://www.tm.agilent.com>. Click "Technical Support". Use "Application Notes" to search for App Note 8510-5A (part number 5956-4352). Although the application note is written for the Agilent 8510 Series Network Analyzers, it also applies to the PNA.

How to set TRL Options

Use one of the following methods:

- In Guided Cal, [Select DUT Connectors and Cal Kits](#) dialog, check Modify Cal. In the Modify Thru Method of Cal dialog box, click View/Modify to invoke the [Modify Calibration Class Assignments](#) dialog box. You can also access this dialog box directly by clicking Calibration, Advanced Modify Cal Kit. These settings determine the default TRL options behavior.
- To override the default TRL behaviors for an Unguided Cal, click **Full TRL 2-PORT**

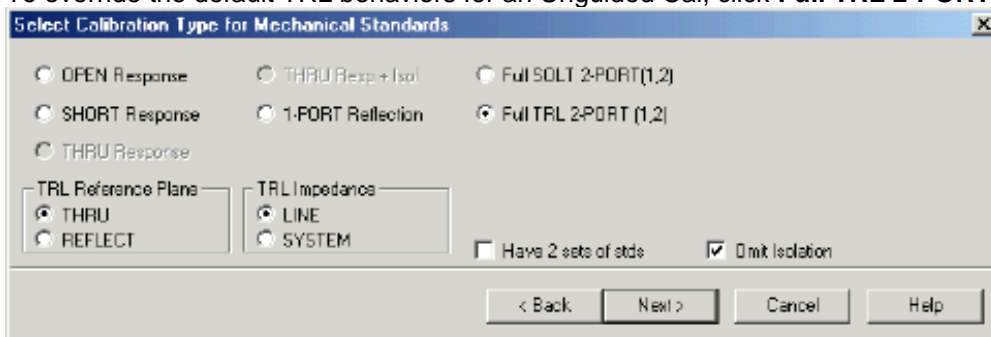

Learn more about using the [front panel interface](#)

Select Calibration Type dialog box help

Note: You can perform a TRL cal only on 2-port PNA models with a dedicated reference receiver for every test port. See [PNA Standard Configurations](#) for a list of model numbers. 4-port PNA models (N5230A Opts 240/245) do NOT support TRL or TRL* calibrations because there is only one reference receiver.

TRL Reference Plane

Thru The THRU standard is used to establish the position of the measurement reference plane. Select if the THRU standard is zero-length or very short.

Reflect The REFLECT standard is used to establish the position of the measurement reference plane. Select if the THRU standard is not appropriate AND the delay of the REFLECT standard is well defined.

TRL Impedance

Line Z0 Specifies that the characteristic impedance of the LINE standard should be used as the system impedance. This ignores any difference between Offset Z0, Offset Loss and system Z0.

System Z0 Transforms the LINE standard impedance and loss to that of the system impedance for use with the calibration error terms. The TRL calibration will first compute the error terms assuming the LINE standard impedance is the system's characteristic impedance (same as LINE option), then modify the error terms to include the impedance transformation. This should only be used with coax since the skin effect model used is a coaxial model.

Learn how to [change System Z0](#).

TRL on a 4-port PNA

Beginning with the PNA code revision 5.25, TRL CAN be performed on a 4-port PNA. Previously, a TRL calibration required a PNA with a reference receiver for every test port. With the new TRL method, a [Delta Match Calibration](#) is first performed or applied.

The accuracy of this TRL cal greatly depends on the accuracy of the Delta Match Calibration. With an accurate Delta Match Calibration, the difference in accuracy between a traditional TRL cal and this TRL cal is negligible.

How to Perform a TRL Cal on a 4-port PNA

1. Click **Calibration, Cal Wizard**.
2. Select a TRL cal kit for the ports to be calibrated.
3. During the calibration, the Cal Wizard [uses a valid Delta Match Cal](#).

Fixture Simulator

The following features allow you to mathematically add (embed) or remove (de-embed) circuits to, or from, your PNA measurements. The mathematical models are applied to specific ports for all measurements on the channel.

For more conceptual information on Fixture Simulation, see "De-embedding and Embedding S-Parameter Networks Using a Vector Network Analyzer". Visit www.Agilent.com and search for **AN 1364-1**.

Note: Before PNA release 5.0, the fixturing features were accessed on the PNA as a macro application.

Fixture Operation Ordering

The test fixturing operations are applied to the measurement results in the following order. This order cannot be changed. Click the following links to learn about each function.

First, Single-ended (2-port) measurement functions


1. [Port Extensions](#)
2. [2-Port De-embedding](#)
3. [Port Z \(Impedance\) Conversion](#)
4. [Port Matching Circuit Embedding](#)
5. [4-Port Network Embed/De-embed](#)

Then, Balanced (4-port) measurement functions

6. [Balanced Conversion](#)
7. [Differential / Common Mode Port Z Conversion](#)
8. [Differential Matching Circuit Embedding](#)

See an [example](#) of how these functions can be used to de-embed unwanted effects of a test fixture, and then mathematically embed the DUT in the circuit in which it is used.

How to select Fixturing Simulator

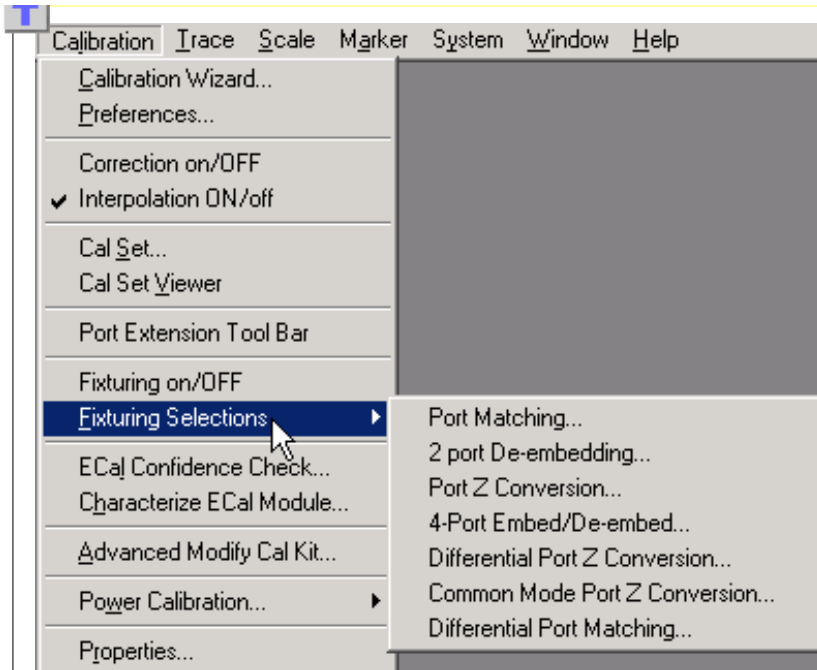


Fixturing ON/off

BOTH of the following must occur to turn a fixturing selection **ON**.

EITHER ONE will turn a fixturing selection **OFF**.

1. Check **Fixturing ON/off** from the above menu.
Port Extensions is NOT affected by Fixturing ON/off.
2. Check **Enable** on the individual fixturing selection dialog box.

Learn more about using the [front panel interface](#)

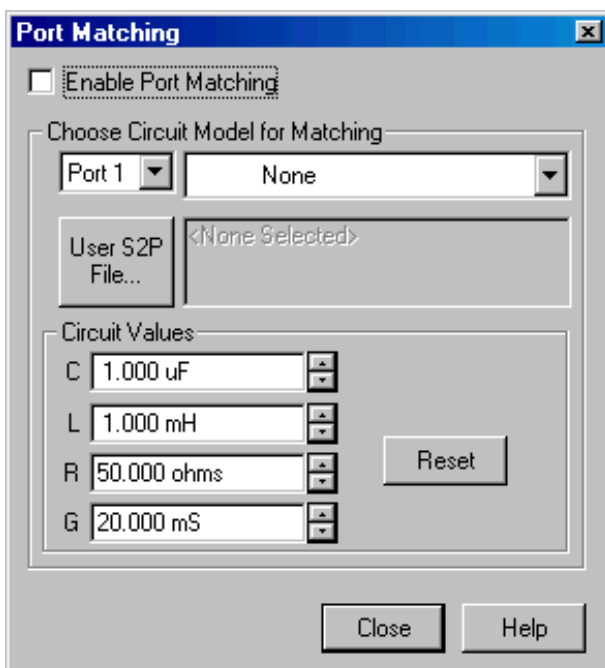

Port Matching dialog box help


This function specifies a circuit to embed (add) to the measurement results.

Enable Port Matching Check to apply the settings to the measurement results. Must also enable Fixturing ON/off.


Port - Select Port in which to apply simulation.

Circuit Model for Matching - Choose one of the following that best emulates your fixture at the selected PNA port:


Series L - Shunt C

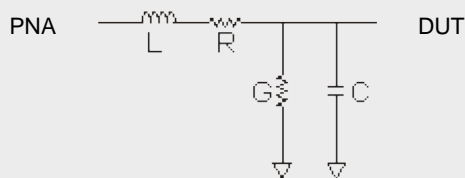


Shunt C - Series L

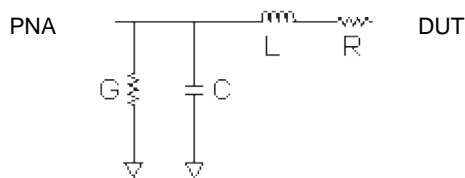


Shunt L - Series C

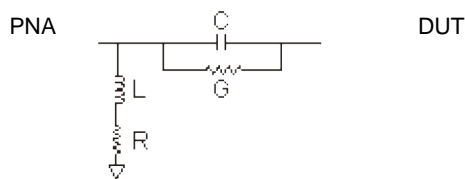

Series C - Shunt L

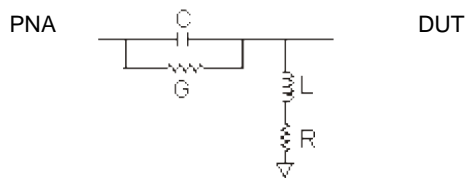

Shunt L - Shunt C

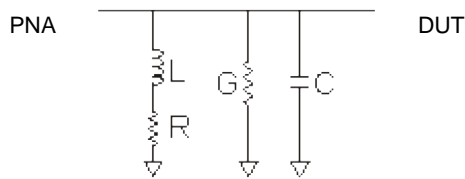

User Defined (S2P File) Load a file that is specified with **User S2P File** button.


None Use no circuit model.

User S2P File Click to specify an S2P file of the circuit model to embed at the selected port. If the normalized impedance value in a recalled User .S2P file is different from the port reference impedance setting of the PNA, the PNA setting is used.

Circuit Values

Capacitance (C), Inductance(L), Resistance(R), Conductance(G) Values for the specific components of the circuit type that models your fixture.

Reset Restores the default values.

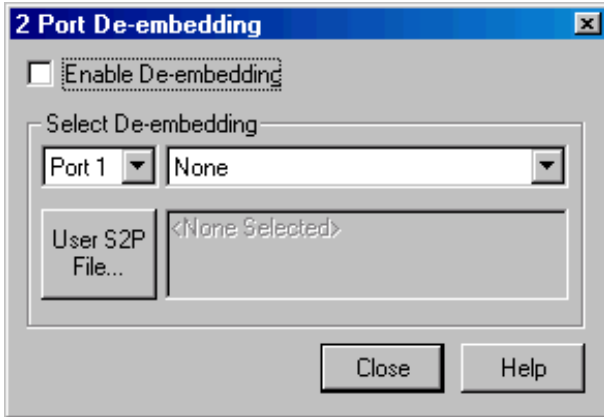

2 Port De-embedding dialog box help


This function **removes** the unwanted effects of a test fixture from the measurement results.

The de-embedding operation recalls an s2p file (Touchstone format) for a 2-port test fixture. The file includes the electrical characteristics of a supplemental fixture or device. The file can be in any standard format (real-imaginary, magnitude-angle, dB-angle) and can represent any 2-port test fixture.

Note: In all cases,

Port 1 of the fixture is assumed to be connected to the PNA

Port 2 of the fixture is assumed to be connected to the DUT.

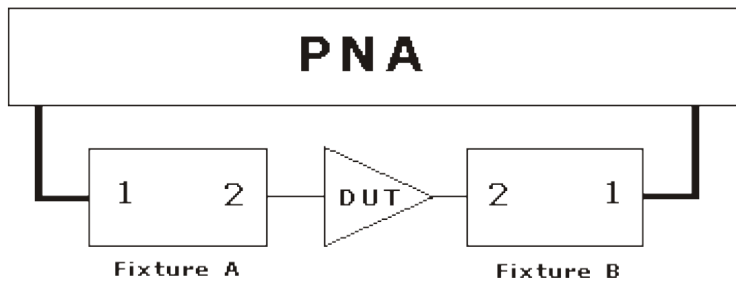


Enable De-embedding Check to apply the settings to the measurement results. Must also enable Fixturing ON/off.

Port - Select Port in which to apply the recalled de-embedding file.

From the drop-down menu, select **User S2P**.

User S2P File Click to specify an existing .S2P file. If the normalized impedance value in a recalled User .S2P file is different from the port reference impedance setting of the PNA, the PNA setting is used.

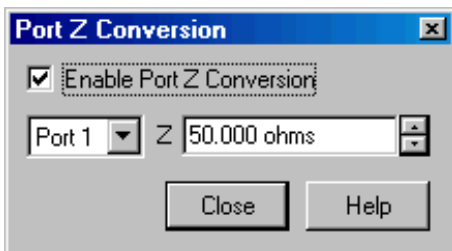

Port Z (Impedance) Conversion dialog box help


This function corrects the measurement and displays the results as if the measurement had been made into the specified impedance value. However, the physical port termination is still approximately 50 ohms.

The specified impedance value is applied to all of the measurements on ONLY the active channel.

Enable Port Z Conversion Check to apply the settings to the measurement results. Must also enable Fixturing ON/off.

Z Resistance part of the desired reference impedance for the specified port and channel.

Close Applies the entries and closes the dialog box

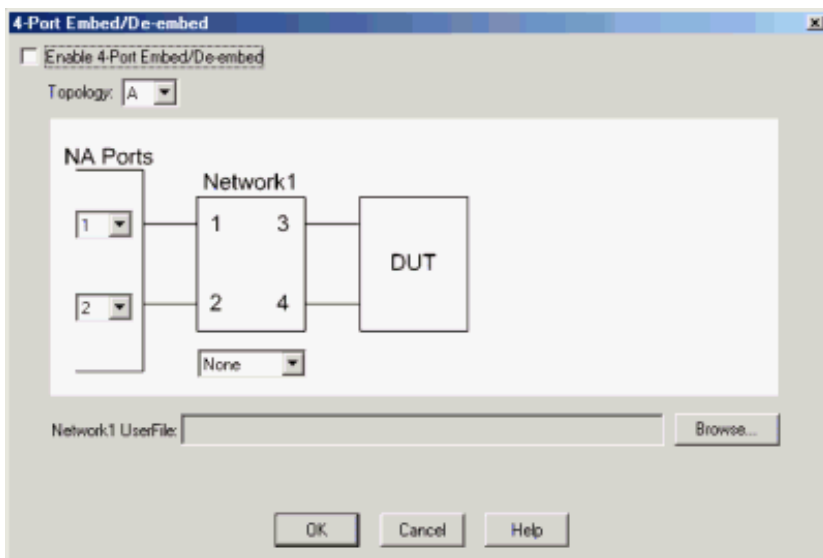

4-Port Embed/De-embed dialog box help

This function specifies a 4-port circuit (*.S4P file) to embed (add) or de-embed (remove) from the measurement results. This selection is used for single-ended and mixed-mode S-parameters. Computation takes place BEFORE Balanced conversion.

There is a single normalized impedance value for each port in the *.S4P file. This impedance value must match the impedance of the previous Port Z setting, or the PNA port impedance.

The PNA will interpolate if the number of data points that are read is different from the current PNA setting.

Enable 4-Port Embed/De-embed Check to apply the settings to the measurement results. Must also enable Fixturing ON/off.

Topology: Select a DUT topology.


- **A** - 2 PNA/DUT Ports
- **B** - 3 PNA/DUT Ports
- **C** - 4 PNA/DUT Ports

Other topology configurations:

1. 4-port DUT; network on one side; None on the other side.


- Specify **Topology C**.

- Use 4-port Network on one side.
- Use 4-port Network on the other side; set to **None**.

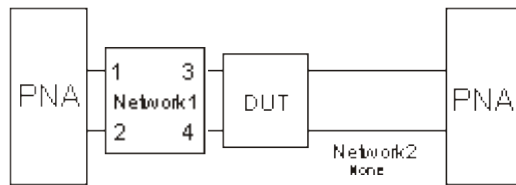

2. 3-port DUT.

- Specify **Topology B**.
- Use 4-port Network1 on one side.
- Use 2-port network on the other side.

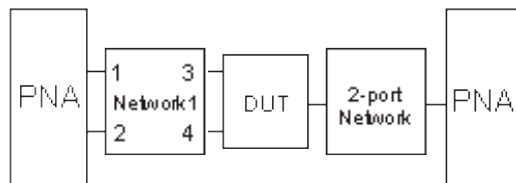

NA Ports - Select the PNA Port that is connected to each circuit port.

Note: The *S4P file always assumes that:
 Network ports 1 and 2 are connected to the PNA
 Network ports 3 and 4 are connected to the DUT


None, Embed, De-embed For Network1 and Network2, select:

- **None** - The same as disabling.
- **Embed** - Add the specified network circuit to the measurement results.
- **De-embed** - Remove the specified network circuit to the measurement results.

Browse For both Network1 and Network2, navigate to find the .*S4P file to embed or de-embed.

OK Applies the changes and closes the dialog box.

Cancel Does NOT apply the changes and closes the dialog box.

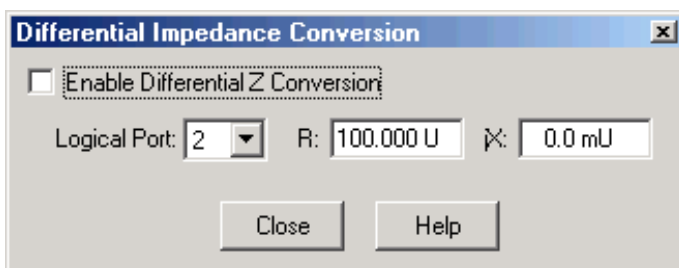

Differential Impedance Conversion dialog box help

This function sets the Differential impedance value for each balanced port.

The default value for **R**: is the SUM of the impedance values for both ports that make the logical port. If Port Z Conversion is not enabled, then System Z0 values for both ports are summed.


Enable Differential Z Conversion Check to apply the settings to the measurement results. Must also enable Fixturing ON/off.

Logical Port Select the logical (balanced) port to receive impedance value. To see logical port numbers, see the measurement topology.

R Real part of the impedance value.

jX Imaginary part of the impedance value.

Close Closes the dialog box.

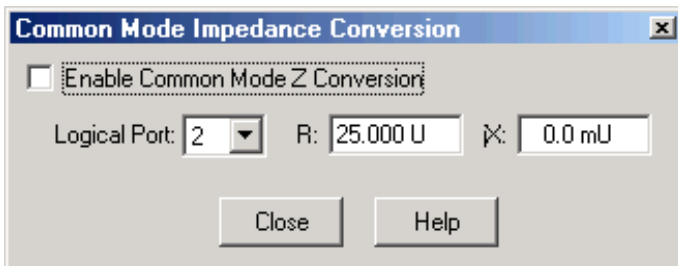

Common Mode Impedance Conversion dialog box help

This function sets Common Mode Impedance value for each balanced port.

The default value for **R**: is calculated as follows.

$$(Z1 * Z2) / (Z1 + Z2)$$

Where ports 1 and 2 comprise the logical port:

Z1 = the Port Impedance values for port 1

Z2 = the Port Impedance values for port 2

If Port Z Conversion is not enabled, then System Z0 values for port 1 and 2 are used in the calculation.


Enable Common Mode Z Conversion Check to apply the settings to the measurement results. Must also enable Fixturing ON/off.

Logical Port Select the logical (balanced) port to receive impedance value. To see logical port numbers, see the measurement topology.

R Real part of the impedance value.

jX Imaginary part of the impedance value.

Close Closes the dialog box.

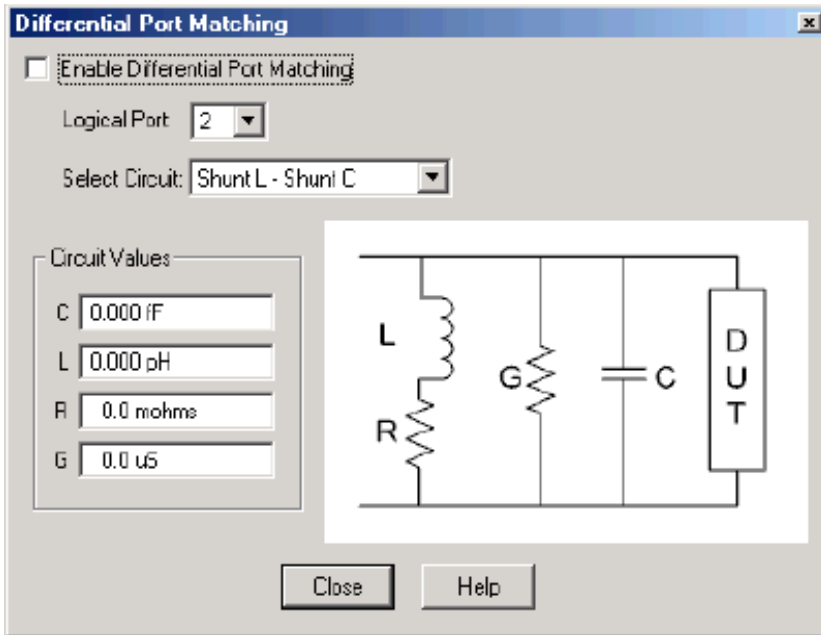

Differential Port Matching dialog box help


This function allows the embedding of a differential matching circuit at a balanced port.

Enable Differential Port Matching Check to embed the selected matching circuit to the measurement results. Must also enable Fixturing ON/off.

Logical Port Choose Logical DUT port to receive the selected matching circuit. To see logical port numbers, see the measurement topology.

Select Circuit Select a matching circuit. Choose from:

- **Shunt L - Shunt C** Predefined circuit.

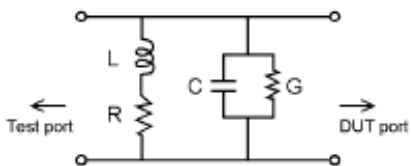

Circuit Values Choose from:

- **C** Capacitance value
 - **G** Conductance value
 - **L** Inductance value
 - **R** Resistance value
- **User defined** Select an *.S2P file that represents the matching circuit. Then click **Browse** to navigate to the *.S2P file.

Note: For the *.S2P file:

Port 1 of the circuit is assumed to be connected to the PNA
 Port 2 of the circuit is assumed to be connected to the DUT.



- **None** No embedded circuit on selected port.

Close Closes the dialog box.

Fixture Simulator Example

The following example shows a DUT and the matching circuit with which the DUT will be used in its intended application. When the DUT is tested in a high-volume manufacturing environment, multiple test fixtures are often required. The most accurate way to test the DUT and ensure measurement consistency between the different test fixtures is to use a simple, repeatable, test fixture without the actual matching elements.

To get the desired performance data, the parasitic effects of the fixture must first be removed (de-embedded) from the measured data. Then a perfect "virtual" matching circuit must be simulated and added mathematically (embedded) to the corrected, measured data. The result is an accurate display of the DUT as though it was actually tested with a physical matching circuit, but without the uncertainties of using real components.

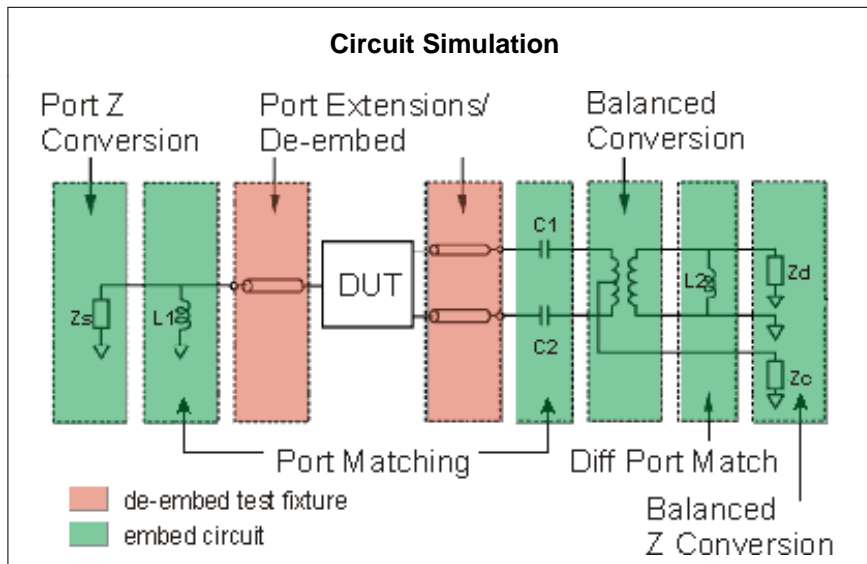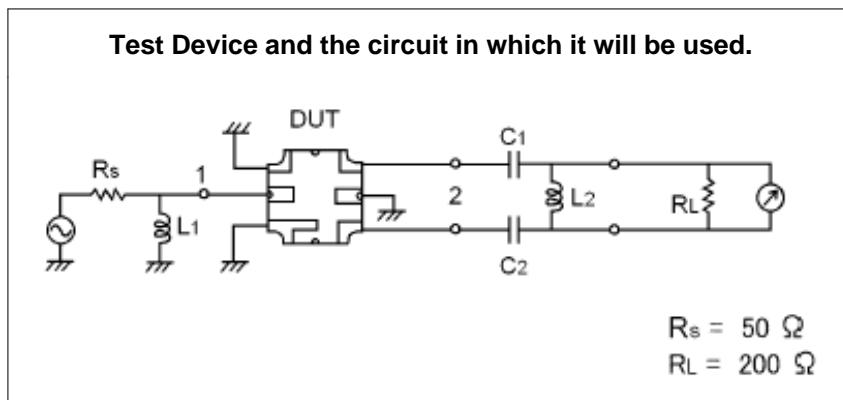

This diagram does NOT refer to the order in which operations are performed.

1. Create a balanced measurement using single-ended to balanced (SE-Bal) topology. Include all relevant measurement settings (IFBW, number of points, and so forth). Once the measurement is created and calibrated, the measurement parameter can be easily changed. For example, Sdd22 to Sds21.

2. Calibrate the measurement at the point where the simple test fixture is connected to the PNA. Use accurate calibration standards and definitions.
3. Remove the effects of the three uncalibrated transmission lines of the simple test fixture. This can be done in several different methods. The easiest is to use manual or automatic port extensions to move the calibration reference plane to the DUT. This removes the electrical length and loss of the fixture's transmission lines, but does not account for fixture mismatch. Another method is to de-embed previously-created *.S2p files of the 3 transmission lines. The files can be created using external ADS modeling software. Another alternative is to create the *.S2P files by independently measuring all 3 ports of the test fixture and saving the results of each to an S2P file.
4. With the test fixture connected to the PNA and a DUT inserted, the measurement results now appear as though calibration was performed at the connections to the DUT, and the device was measured in a 50-ohm single-ended test environment. The following steps will cause the results to reflect the performance of the device as though the device is embedded in the circuit in which it will be used.
5. Port 1 of the device is a single-ended port and sees a source impedance the same as the PNA system impedance, so no change is required. However, if R_s were a value other than 50 ohms, Port 1 Impedance Conversion would be used to simulate the different impedance.
6. Port Matching is used to simulate L1 inductance. Select any of the Shunt L circuits to embed (add) to the measurement results. Enter the value of L and R. The C and G values can be entered as 0 (zero).
7. Port Matching is used to simulate C1 and C2 capacitance. For both port 2 and port 3, select any of the **Series C** circuits to embed (add) to the measurement results. Enter the value of C and G. The L and R values can be entered as 0 (zero).
8. Balanced Conversion mathematically simulates the measurement in balanced mode.
9. Differential Port Matching is used to simulate L2 inductance. Select Shunt L- Shunt C and enter the inductance / resistance value. The C and G values can be entered as 0 (zero).
10. Finally, Differential Z Conversion is used to simulate a circuit termination of 200 ohms. If you are making Common Mode measurements, specify Common Mode Z Conversion.

Markers

The Markers function provides a numerical readout of measured data, a search capability for specific values, and can change stimulus settings. There are 9 regular markers and one Reference marker available per trace. This topic discusses all aspects of markers.

Note: Marker Readout can be turned ON / OFF and customized from the **View** menu. See [Marker Readout](#)

Creating and Moving Markers

Delta Markers

Searching with Markers

Marker Functions (Change Instrument Settings)

Advanced Marker Settings


Marker Table

Other Analyze Data topics


How to Create and Move Markers

Use one of the following methods:


- Active Entry toolbar



- Marker toolbar

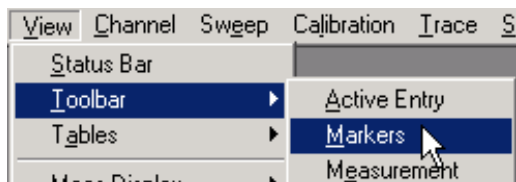


- Marker dialog box



Learn more about using the [front panel interface](#)

Create a Marker


- From the Active Entry toolbar, press a marker number. To access markers 4 through 9, press  repeatedly.
- From the Marker Toolbar or Marker Dialog Box, select a marker number and click **ON**

Moving a Marker

To move a marker, make the marker active by selecting its number (in any of the previous 3 methods). Then change the stimulus value using any of the following methods:

- Type a value
- Scroll to a stimulus value using the up / down arrows
- Click the stimulus box, then use the front-panel knob.

Note: To change marker properties, the marker must be active. The **active marker** appears on the analyzer display as \tilde{N} . All of the other markers are inactive and are represented on the analyzer display as D.

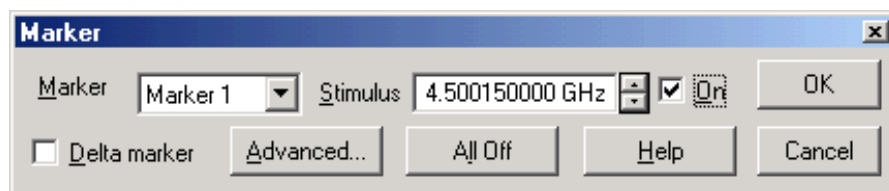

Marker dialog box help

Marker Specifies the marker number that you are defining.

Stimulus Specifies the X-axis value of the selected marker. To change stimulus value, type a value, use the up and down arrows, or click in the text box and use the front-panel knob.

On Check to display the marker and corresponding data on the screen.

Delta Marker Check to make the specified marker data relative to the reference marker. If not already on, the reference (R) marker will be displayed automatically. [Learn more about Delta Markers](#)

Advanced... Invokes the [Advanced Markers](#) dialog box.

All Off Switches OFF all markers on the active trace.

Delta Markers

Delta Markers allow you to view data that is relative to the **reference** marker.

A delta marker can be set from the [Marker dialog box](#) or the [Marker Toolbar](#).

When a Delta marker is created, the reference marker will be activated automatically.



Searching with Markers

You can use markers to search measurement data for specific criteria.

If there is no valid data match for any of the search types, the marker will not move from its current position.


How to Search with Markers

Use one of the following methods:

- 
- 

Only **Max**, **Min**, **Left Peak**, and **Right Peak** search types are available from Active Entry Keys

Learn more about using the [front panel interface](#)

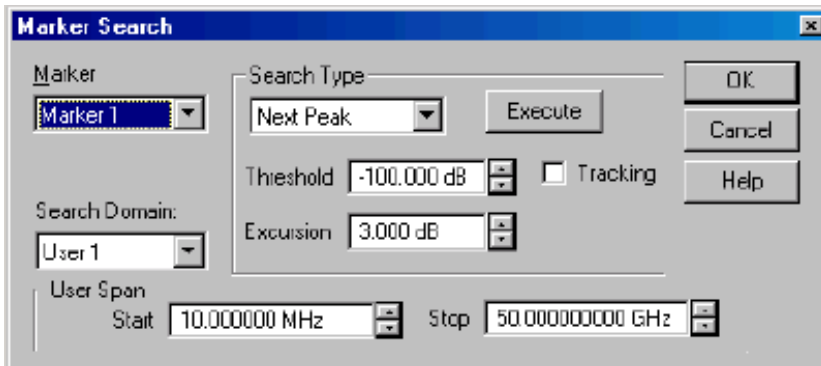

Marker Search dialog box help

Marker Specifies the marker that you are defining.

Search Domain Defines the area where the marker can move or search. For full span, the marker searches for specified values within the full measurement span. For user span, the marker searches for specified values within a measurement span that you define. [Learn more about Search Domain.](#)

Search Type

Maximum Marker locates the maximum (highest) data value.

Minimum Marker locates the minimum (lowest) data value.

Next Peak Marker locates the peak with the next lower amplitude value relative to its starting position. See [What is a Peak.](#)

Peak Right The marker locates the **next valid peak to the right** of its starting position on the X-axis .See [What is a Peak.](#)

Peak Left The marker locates the **next valid peak to the left** of its starting position on the X-axis .See [What is a Peak.](#)

- **Threshold** - Minimum amplitude (dB). To be considered valid, the peak must be **above** the threshold level. The valley on either side can be below the threshold level. [Learn more...](#)
- **Excursion** The vertical distance (dB) between the peak and the valleys on both sides. To be considered

a peak, data values must "fall off" from the peak on both sides by the excursion value. [Learn more...](#)

Target Enter the Target value. The marker moves to the first occurrence of the Target value **to the right of its current position**. Subsequent presses of the Execute button cause the marker to move to the next value to the right that meets the Target value. When the marker reaches the upper end of the stimulus range, it will "wrap around" and continue the search from the lower end of the stimulus range (left side of the window).

- If **Discrete Marker** is OFF, the marker locates the interpolated data point that equals the target value.
- If **Discrete Marker** is ON and there are two data points on either side of the target value, the marker locates the data point closest to the Target value

Bandwidth Marker1 locates the highest peak which falls off on both sides by the specified level. (When Bandwidth is selected, a Level box appears to specify the level in dB down from the peak where bandwidth is measured - default is -3dB.)

This search type always uses Markers 1-4.

- Marker 1: Peak
- Marker 2: Specified level down to the left of the peak
- Marker 3: Specified level down to the right of the peak
- Marker 4: Center frequency of the bandwidth

Display readout for Bandwidth Search:

- **BW:** (Marker 3 x-axis value) - (Marker 2 x-axis value) = width of the filter
- Center Mathematical midpoint between markers 2 and 3
- Q Ratio of Center Frequency to Bandwidth (Center Frequency / Bandwidth)
- Loss Y-axis value of Marker 4. This is the loss of the filter at its center frequency. The ideal filter has no loss (0 dB) in the passband.

Note: You must either press **Execute** or check **Tracking** to initiate all search types.

Execute Click to cause the marker to search for the specified criteria.

Tracking Check to cause the marker to search for the specified criteria with each new sweep. The searches begin with the first sweep after Tracking has been checked, based on the current search type and domain information. Therefore, make sure that the search criteria are in the desired state before using the data. You cannot manually change the stimulus setting for a marker if Tracking is selected for that marker.

What Is a "Peak"?

You define what the analyzer considers a "peak" by selecting the following two peak criteria settings:

- **Threshold** - Minimum amplitude (dB). To be considered valid, the peak must be **above** the threshold level. The valley on either side can be below the threshold level.
- **Excursion** - The vertical distance (dB) between the peak and the valleys on both sides. To be considered a peak, data values must "fall off" from the peak on both sides by the excursion value.


Example:

Threshold Setting: -10dB

Excursion Setting: 1dB

Scale = 1 dB / Division

Mouse over the graphic to find a valid peak.

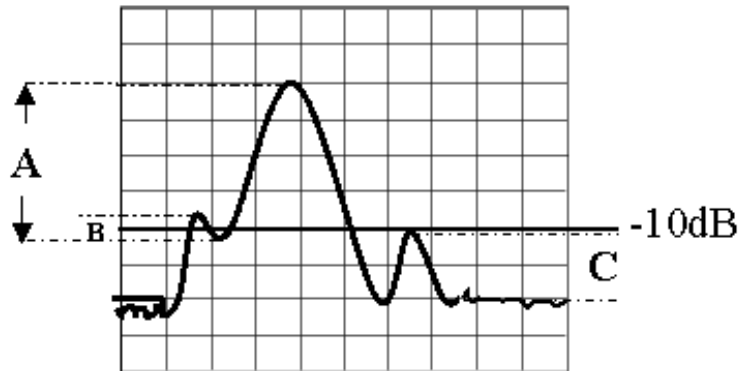


- **Peak A** = Valid Peak (Above Threshold and Excursion Settings)
- **Peak B** = Invalid Peak (Below Excursion Setting)
- **Peak C** = Invalid Peak (Below Threshold Setting)

Search Domain

Search domain settings restrict the stimulus values (X-axis for rectangular format) to a specified span. Set the Start and Stop stimulus settings of these **User** spans. If Start is greater than Stop, the marker will not move.

- The default domain of each new marker is "full span".
- There are 16 user-defined domains for every channel.
- The user-defined domains can overlap.
- More than one marker can use a defined domain.

The graphic below shows examples of search domains.

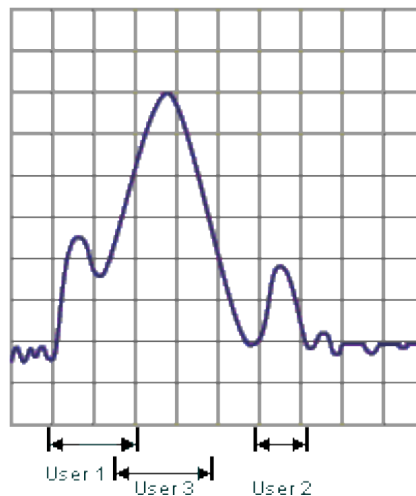


Marker Functions - Change Instrument Settings


The following settings change the relevant PNA settings to the position of the active maker.

How to change instrument setting using markers

Use one of the following methods:



-




-

Only **Center**, **Ref Level**, and **Delay** are available

- From the Marker Toolbar only Start, Stop Center and Span Frequencies are available.

Learn more about using the [front panel interface](#)

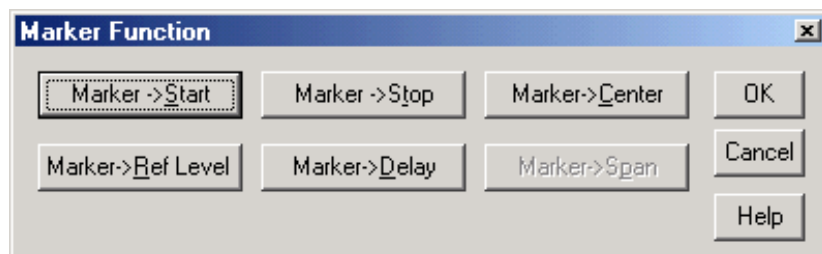

Marker Function dialog box help

Note: Marker Functions do not work with channels that are in CW or Segment Sweep mode.

Marker =>Start Sets the start sweep setting to the value of the active marker.

Marker =>Stop Sets the stop sweep setting to the value of the active marker.

Marker =>Center Sets the center of the sweep to the value of the active marker.


Marker =>Ref Level Sets the screen reference level to the value of the active marker.

Marker =>Delay The phase slope at the **active marker** stimulus position is used to adjust the line length to the receiver input. This effectively flattens the phase trace around the active marker. (Additional Electrical Delay adjustments are required on devices without constant group delay over the measured frequency span.) You can use this to measure the electrical length or deviation from linear phase.

This feature adds phase delay to a variation in phase versus frequency; therefore, it is only applicable for ratioed measurements. (See Measurement Parameters.)


Marker =>Span Sets the sweep span to the span that is defined by the delta marker and the marker that it references. Unavailable if there is no delta marker.

How to select Advanced Marker settings



Then click **Advanced** on the Marker dialog box

Learn more about using the [front panel interface](#)

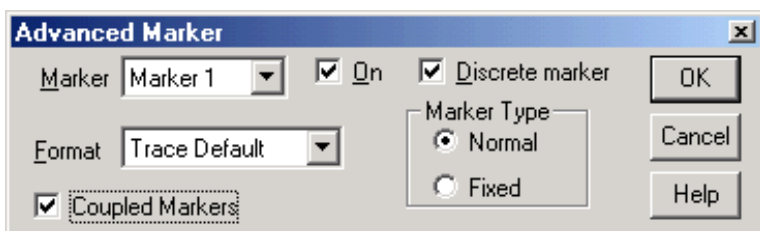

Advanced Marker dialog box help

Marker Specifies the marker number that you are defining.

On Check to display the marker and corresponding data on the screen.

Format Displays the marker data in a format that you choose. The marker format could be different from the grid format. In the default setting, the marker and grid formats are the same.

Discrete Marker Check to display values at only the discrete points where data is taken. Clear to display values that are interpolated from the data points.

Coupled Markers Check to couple markers by marker number, 1 to 1, 2 to 2 and so forth. The markers will remain coupled until this box is unchecked. [Learn more about coupled markers.](#)

Marker Type

Normal Has a fixed stimulus position (X-axis) and responds to changes in data amplitude (Y-axis). It can be scrolled left and right on the X-axis by changing the marker stimulus value. Use this marker type with one of the marker search types to locate the desired data.

Fixed Has a fixed X and Y-axis position based on its placement on the trace when it was set to fixed. It does NOT move with trace data amplitude. It can be scrolled left and right on the X-axis by changing the marker stimulus value.


Use this marker type to quickly monitor "before and after" changes to your test device. For example, you could use fixed markers to record the difference of test results before and after tuning a filter.

Coupled Markers

The coupled markers feature causes markers on different traces to line up with the markers on the selected trace. Markers are coupled by marker number, 1 to 1, 2 to 2, 3 to 3, and so forth. If the x-axis domain is the same (such as frequency or time), coupling occurs across all channels, windows, and traces. Trace markers in a different x-axis domain will not be coupled. If a trace marker has no marker to couple with on the selected trace, the marker remains independent.

Coupled Markers Model

This model simulates the use of coupled markers in the PNA

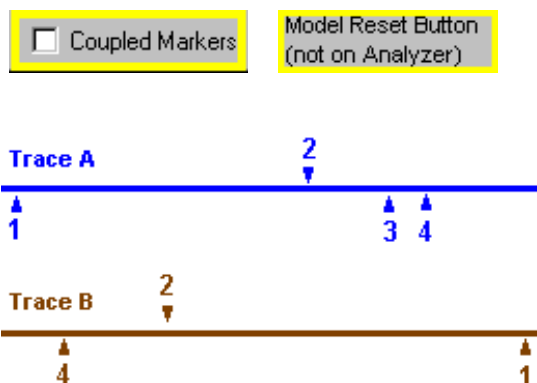

1. Click **Trace A** or **Trace B**
2. Click **Coupled Markers**
3. Notice the following:
 - * Markers on the unselected trace move to the x-axis position of the selected trace.
 - * If a marker number on the unselected trace has no corresponding marker on the selected trace, no movement occurs for that marker.
4. Click **Reset** to run the model again. (There is no Reset for coupled markers on the PNA.)


Set Coupled Markers from the [Advanced Markers](#) dialog box.


Marker Table

You can display a table that provides a summary of marker data for the active trace. The marker data is displayed in the specified format for each marker.

How to view the Marker Table

Use one of the following methods:

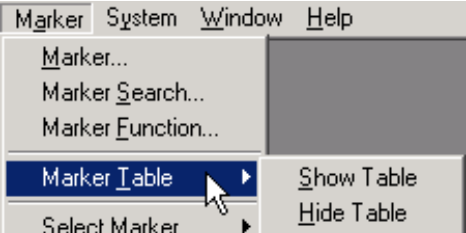- 

The screenshot shows a menu with the following items: Marker..., Marker Search..., Marker Function..., Marker Table, and Select Marker. The Marker Table item is highlighted, and a sub-menu is open showing 'Show Table' and 'Hide Table' options.
- 

The screenshot shows a 'Marker Table' button followed by a plus sign and four function keys: F1 (yellow), F2 (green), F3 (blue), and F4 (purple).

Learn more about using the [front panel interface](#)

Note: The Marker Table and Marker Readout can also be turned on from the **View** menu. (See [Customize Your Analyzer Screen.](#))

Manipulate Data Using Math Operations

You can perform four types of math on the active trace and a memory trace. In addition three statistics (Mean, Standard Deviation and Peak to Peak) can be calculated and displayed for the active data trace.

Trace Math

Trace Statistics

Other Analyze Data topics

Trace Math


To perform any of the math operations, you must first store a trace to memory. You can display the memory trace using the View options.

Trace math is performed on the complex data before it is formatted for display. See the [PNA data processing map](#).


Markers can be used while viewing the memory trace.

How to select Trace Math

Use either of the following methods:



•




•



Only the following are available from Active Entry

- **Data>>Mem** (stores Data trace into Memory)
- **Data/Mem** (performs math operation: Data divided by memory)
- **Data** (displays data trace with no math operation applied)
- **Mem on/OFF** (turns Memory trace on or off)

Learn more about using the [front panel interface](#)

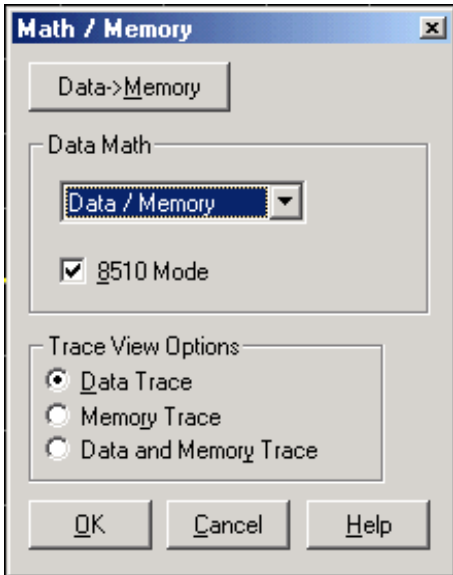

Math / Memory dialog box help

Data=>Memory Puts the active data trace into memory.

Data Math

Data Does no mathematical operation.

Data / Memory - Current measurement data is divided by the data in memory. Use for ratio comparison of two traces, such as measurements of gain or attenuation.

Data – Memory - Data in memory is subtracted from the current measurement data using vector subtraction on complex measurement data. For example, you can use this feature for storing a measured vector error, then subtracting this error from the DUT measurement.


Data + Memory - Current measurement data is added to the data in memory.

Data * Memory - Current measurement data is multiplied by the data in memory.

Learn more about Data * Memory and Data + Memory

8510 Mode Check to simulate the Agilent 8510 data processing chain as it pertains to Trace Math and Memory. This setting applies to all channels. When the box is checked or cleared, the PNA performs an Instrument Preset and retains its setting through subsequent Instrument Presets.

This setting is saved as part of an instrument state. However, when recalled, this setting is assumed only temporarily. When a subsequent PNA Preset is performed, the PNA reverts to the setting that was in effect before the state was recalled.

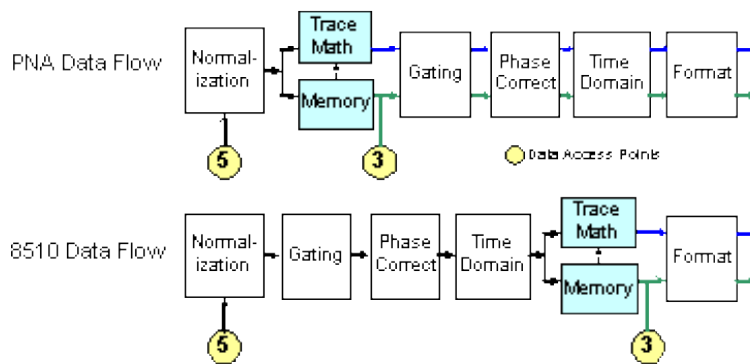

This graphic represents the relevant portion of the data flow. See the entire PNA data processing chain.

Trace View Options

Data Trace Displays the current measurement trace only.

Memory Trace Displays the trace that was put in memory only.

Data and Memory Trace Displays both the current measurement trace and the trace that was put in memory.

[Learn more about Trace Math](#) (scroll up)

Data * Memory and Data + Memory

Use **Data * Memory** and **Data + Memory** to perform math on an active data trace using data from your own formulas or algorithms rather than data from a measurement. For example, if you want to simulate the gain of a theoretical amplifier placed in series before the DUT, you could:

1. Create an algorithm that would characterize the frequency response of the theoretical amplifier.
2. Enter complex data pairs that correspond to the number of data points for your data trace.
3. Load the data pairs into memory with SCPI or COM commands. The analyzer maps the complex pairs to correspond to the stimulus values at the actual measurement points.
4. Use the **data + memory** or **data * memory** function to add or multiply the frequency response data to the measured data from the active data trace.

Note: The data trace must be configured before you attempt to load the memory.

Trace Statistics

You can calculate and display statistics for the active data trace. These statistics are:

- Mean
- Standard deviation
- Peak-to-peak values

You can calculate statistics for the full stimulus span or for part of it with user ranges.


There are **16** user ranges per channel. These user ranges are the same as the search domains specified for a marker search in that same channel; they use the same memory registers and thus share the same stimulus spans. If you specified search domains with marker search for a channel, you can recall these same spans by selecting the corresponding user ranges. The user ranges for a channel can overlap each other.

A convenient use for trace statistics is to find the peak-to-peak value of passband ripple without searching separately for the minimum and maximum values.


The trace statistics are calculated based on the format used to display the data.

- Rectangular data formats are calculated from the scalar data represented in the display
- Polar or Smith Chart formats are calculated from the data as it would be displayed in Log Mag format

How to activate Trace Statistics

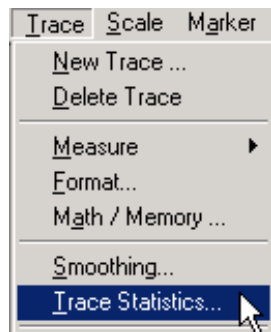

Learn more about using the [front panel interface](#)

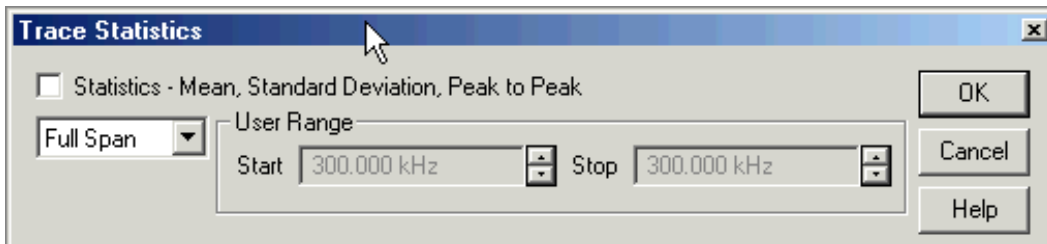

Trace Statistics dialog box help

Statistics Check to display mean, standard deviation, and peak to peak values for the active trace.

Full Span Specifies the span where data is collected for a statistical math operation. You can define up to **16** user ranges per channel. You can also define the user ranges from the [Marker Search dialog box](#).

Start Defines the start value of the selected user range.

Stop Defines the stop value of the selected user range.

[Learn more about Trace Statistics](#) (scroll up)

Use Limits to Test Devices

Limit lines allow you to compare measurement data to performance constraints that you define.

[Overview](#)

[Create and Edit Limit Lines](#)

[Display and Test with Limit Lines](#)

[Testing with Sufficient Data Points](#)

Other Analyze Data topics

Overview

Limit lines are visual representations on the PNA screen of the specified limits for a measurement. You can use limit lines to do the following:

- Give the operator **visual guides** when tuning devices.
- Provide **standard criteria** for meeting device specification.
- Show the **comparison** of data versus specifications.

Limit testing compares the measured data with defined limits, and provides optional **Pass or Fail** information for each measured data point.

You can have up to **100** discrete lines for each measurement allowing you to test all aspects of your DUT response.

Limit lines and limit testing are NOT available with **Smith Chart** or **Polar** display format. If limit lines are ON and you change to Smith Chart or Polar format, the analyzer will automatically disable the limit lines and limit testing.

Note: Limit Lines are NOT currently supported on the [Frequency Converter Application](#). They CAN be used on basic [Frequency Offset](#) measurements.



Create and Edit Limit Lines

You can create limit lines for all measurement traces. The limit lines are the same color as the measurement trace.







Limit lines are made up of discrete lines with four coordinates:

- BEGIN and END stimulus - X-axis values.
- BEGIN and END response - Y-axis values.

How to create and edit Limit Lines

Limits are created, edited, and activated, with the limit table.

Use one of the following methods to show the limit table:

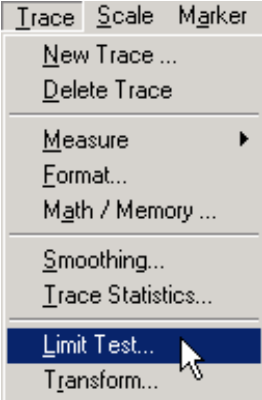-  +    
- 
 - Trace
 - Scale
 - Marker
 - New Trace ...
 - Delete Trace
 - Measure
 - Format...
 - Math / Memory ...
 - Smoothing...
 - Trace Statistics...
 - Limit Test...**
 - Transform...

Learn more about using the [front panel interface](#)

Limit Table

	TYPE	BEGIN STIMULUS	END STIMULUS	BEGIN RESPONSE	END RESPONSE
1	MIN	1.930000 GHz	1.990000 GHz	-5.000000 dB	-5.000000 dB
2	MAX	1.000000 GHz	1.900000 GHz	-60.000000 dB	50.000000 dB
3	MAX	2.050000 GHz	3.000000 GHz	-50.000000 dB	-60.000000 dB
4	OFF	<input type="checkbox"/>	0.000000 Hz	0.000000 dB	0.000000 dB

Note: To ADD a limit line to the table, change the last limit line to either MAX or MIN

1. In the **Type** area of the Limit Table, select **MIN** or **MAX** for Limit Line 1.
The MIN value will fail measurements BELOW this limit.
The MAX value will fail measurements ABOVE this limit.
2. Click **BEGIN STIMULUS** for Limit Segment 1. Enter the desired value.
3. Click **END STIMULUS** for Limit Segment 1. Enter the desired value.
4. Click **BEGIN RESPONSE** for Limit Segment 1. Enter the desired value.
5. Click **END RESPONSE** for Limit Segment 1. Enter the desired value.
6. Repeat Steps 1-5 for each desired limit line.

Displaying and Testing with Limit Lines

After creating limit lines, you can then choose to **display** or **hide** them for each trace. The specified limits remain valid even if limit lines are not displayed.

Limit testing cannot be performed on memory traces.

You can choose to provide a visual and / or audible PASS / FAIL indication.

With limit testing turned ON:


- Any portion of the measurement trace that **fails** is **displayed in red**.
- Any portion of the measurement trace that does **NOT fail** remains unchanged and silent.

PASS is the default mode of Pass / Fail testing. A data point will FAIL only if a measured point falls outside of the limits.


- If the limit line is set to OFF, the entire trace will PASS.
- If there is no measured data point at a limit line stimulus setting, that point will PASS.

How to display and test with Limit Lines

The following method Invokes a dialog box

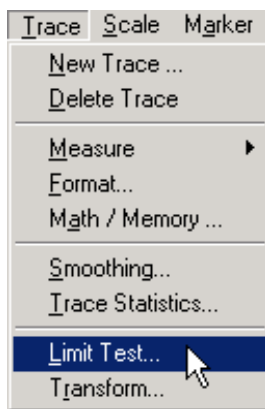


The following method shows the Limit Table and provides Test ON/OFF and Line ON/OFF capability.



Sound ON Fail selection is not available from the Active Entry

Learn more about using the front panel interface

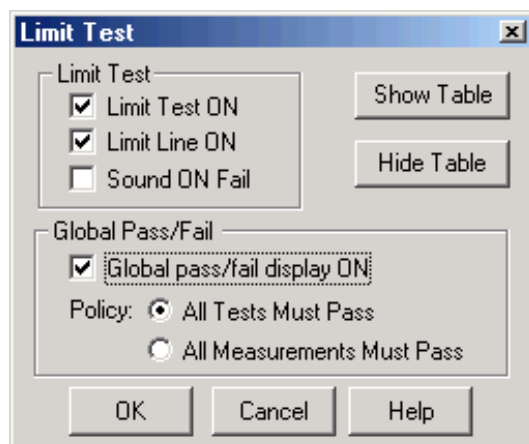

Limit Test dialog box help

Limit Test

Limit Test ON Check the box to compare the data trace to the limits and display PASS or FAIL.

Limit Line ON Check the box to make the limits visible on the screen. (Testing still occurs if the limits are not visible.)

Sound ON Fail Check the box to make the PNA beep when a point on the data trace fails the limit test.

Global Pass/Fail

The Pass/Fail indicator provides an easy way to monitor the status of all measurements.

Global pass/fail display ON Check to display the Global Pass/Fail status.

Policy: Choose which of the following must occur for the Global Pass/Fail status to display PASS:

- All Tests (with **Limit Test ON**) Must Pass - This setting reads the results from the Limit Tests. If all tests (with **Limit Test ON**) PASS, then the Global Pass/Fail status will PASS.
- All Measurements Must Pass - This more critical setting shows FAIL unless all measured data points fall within established test limits and Limit Test is ON. **Note:** With this selection, all Limit Tests could PASS, yet the Global Pass/Fail status show FAIL. This is because Limit Tests default to Pass and Global Pass/Fail with 'All Measurements Must Pass' selected defaults to FAIL.

Show Table Shows the table that allows you to create and edit limits.

Hide Table Makes the limits table disappear from the screen.

Note: To ADD a limit line to the table, change the last limit line to either MAX or MIN


[Learn more about displaying and testing with Limits \(scroll up\)](#)

Testing with Sufficient Data Points


Limits are checked only at the actual measured data points. Therefore, It is possible for a device to be out of specification without a limit test failure indication if the data point density is insufficient.

The following image is a data trace of an actual filter using 11 data points (approximately one every vertical graticule). The filter is being tested with a minimum limit line (any data point under the limit line fails).

Although the data trace is clearly below the limit line on both sides of the filter skirts, there is a PASS indication because there is no data point being measured at these frequencies.

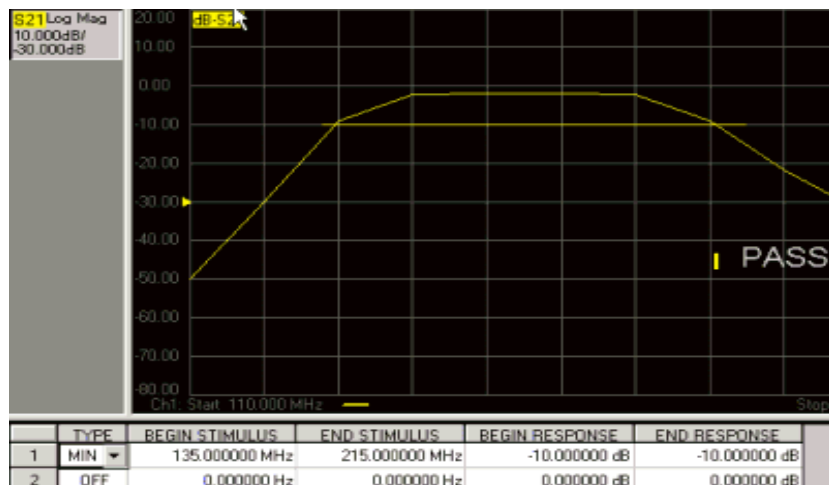

The following image shows the exact same conditions, except the number of data points is increased to 1601. The filter now fails the minimum limit test indicated by the red data trace.

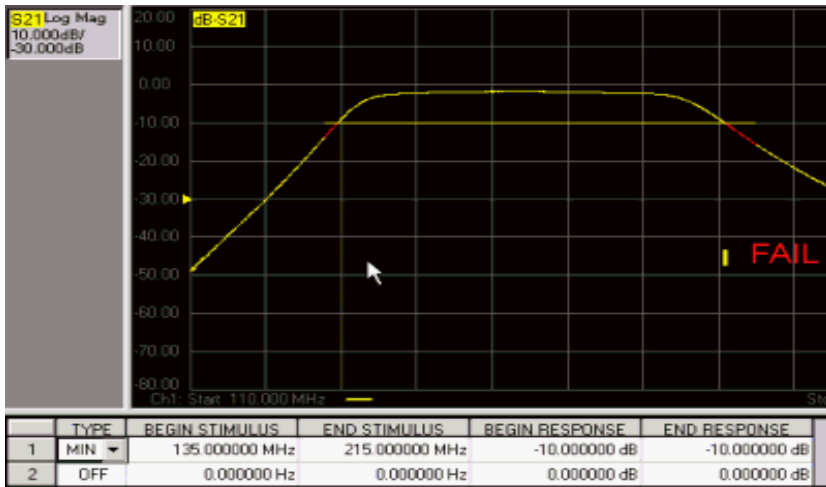

Save and Recall a File

The PNA allows you to save and recall files to and from an internal or external storage device in a variety of file formats.

[How to Save a File](#)

[How to Recall a File](#)

[Instrument / Calibration State Files \(.cst, .sta, .cal, .csa\)](#)

[Measurement Data Files \(.prn, .SnP, .cti\)](#)


[Define Data Saves](#)

[Managing Files without a Mouse](#)

Other Data Outputting topics

How to Save a File

Use one of the following methods:

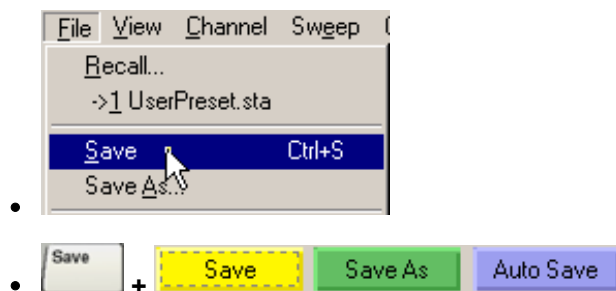


Save Immediately saves the PNA state and possibly calibration data to the filename and extension you used when you last performed a Save. Only .cst, .sta, and .csa files are remembered when Save is performed. This file will be overwritten the next time you click **Save**. To prevent this, use one of the following methods.

Save As Invokes the Save As dialog box.

Auto Save (Only available from the Active Entry keys) Saves state and calibration data to the internal hard disk in the C:\Program Files\Agilent\Network Analyzer\Documents folder. A filename is generated automatically using the syntax "atxxx.cst"; where xxx is a number that is incremented by one when a new file is Auto Saved.

Note: You can NOT save Frequency Converter Application .S2P files using this method. To learn how, see [Using FCA, Save Data](#).

Learn more about using the [front panel interface](#)

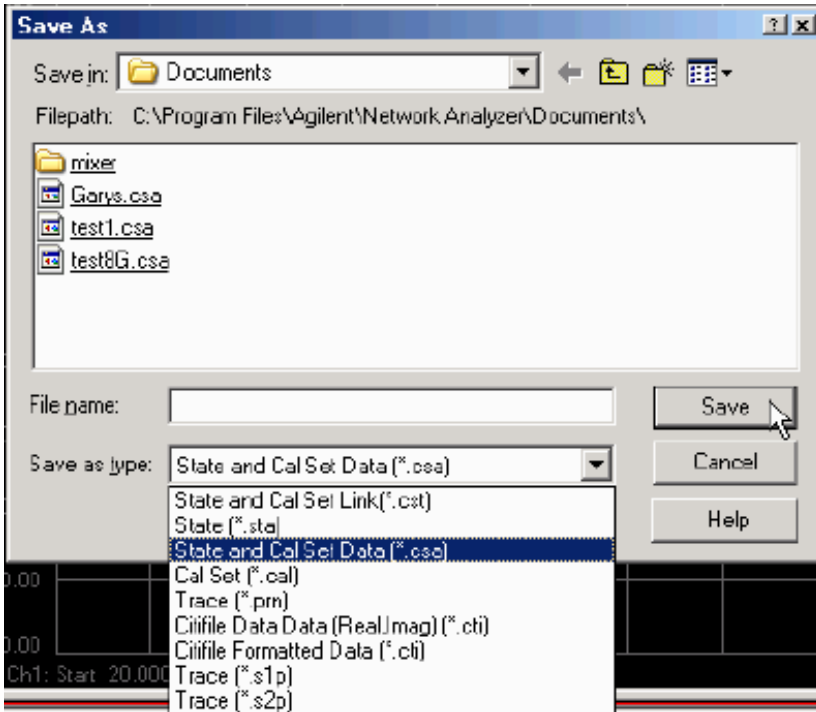

Save As dialog box help

Save in Allows you to navigate to the directory where you want to save the file.

File name Displays the filename that you either typed in or clicked on in the directory contents box.

Save as type

The following file types save **Instrument states and Calibration data**. These file types are only recognized by Agilent PNA Series analyzers. [Learn more about these file types.](#)

- *.cst - save Instrument state and a reference pointer to the Cal Set data.
- *.csa - save Instrument state and actual Calibration data (cal/state archive)
- *.sta - save Instrument state ONLY (**no** calibration data)
- *.cal - save actual Calibration data ONLY (**no** Instrument state)

Note: Before saving a .cst file (Instrument State and Calibration data), be sure that a User Cal Set is being used for the calibration; not a Cal Register. When a **.cst file** is created, a "pointer" to the Cal Set is also saved. Cal Registers are overwritten with new data whenever a calibration is performed, and may not be accurate cal data when the .cst file is recalled. [Learn more about Cal Sets.](#)

The following file types save **Measurement data** for use in spreadsheet or CAE programs. Click to learn more about these file types.




- [*.prn](#)
- [*.s1p](#) , [*.s2p](#), [*.s3p](#), [*.s4p](#)
- [*cti \(citifile\)](#)

Note: To save the PNA screen as .bmp, .jpg, or .png graphics file types, click **File / Print to File**. [Learn more.](#)


Save Saves the file to the specified file name and directory.

How to Recall (open) a file

Use one of the following methods:

- 
The screenshot shows a menu bar with 'File', 'View', 'Channel', and 'Sweep'. The 'File' menu is open, showing 'Recall...' (highlighted), 'Save', and 'Ctrl+S'.
- Press  repeatedly, then 

Learn more about using the [front panel interface](#)

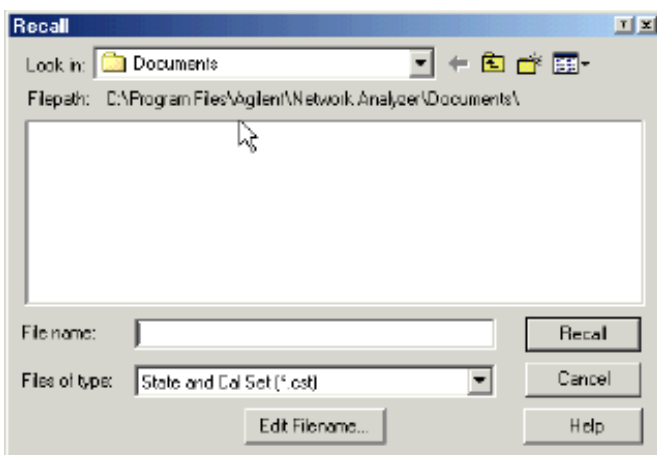

Recall dialog box help

Look in Allows you to select the directory that contains the file that you want to recall.

File name Displays the filename that you either typed in or clicked on in the directory contents box.

Files of type Allows you view and select files that are listed in categories of a file type.

Recall Recalls the file displayed in the file name box.

Note: *.s1p, *.s2p, *.s3p files cannot be recalled by the PNA.

Instrument State / Calibration Files

You can save, and later recall, instrument setups (states) and calibration data.

An **Instrument State** contains almost every PNA setting. The following PNA settings are NOT saved and recalled with Instrument State:

- [GPIB address](#)
- [RF power ON/OFF](#)
- [Test set I/O settings](#)

File Types

The following file types are used to save and recall calibration and instrument states:

- ***.cst** files contain both instrument state AND a reference pointer to a Cal Set file which contains the actual calibration data. Using a *.cst file is the **quickest and most flexible** method of saving and recalling a calibrated instrument state. Because only a reference to the Cal Set is saved, the Cal Set can be shared with other measurements. However, if the Cal Set is changed or deleted, the calibration will no longer be valid when the *.cst file is recalled. [Learn more about Cal Sets](#).
- ***.csa** files contain both instrument state AND actual calibration data, not a reference pointer to the Cal Set. This is the **safest** method of saving and recalling a calibrated instrument state. However, the file size is larger than a *.cst file, and the save and recall times are longer. In addition, because the actual calibration data is saved, it is very difficult to share the cal data with other measurements.

Note: An **Overwrite calset data?** dialog will appear when the following sequence occurs:

1. A *.csa file was saved with a User Cal Set in use. This would occur if the calibration was saved as a User Cal Set, or if a User Cal Set had been applied to the channel. [See Using Cal Sets](#).
2. The User Cal Set was changed sometime after the *.csa file save.
3. The *.csa file is recalled.

The message indicates that the User Cal Set will be overwritten with the older *.csa cal data. You can choose **OK** to overwrite the data or **Cancel** to abort the recall.

- ***.sta** files contain ONLY instrument state data; no cal data or reference to the Cal Set.
- ***.cal** files contain ONLY actual calibration data; no instrument state data.

Measurement Data Files

Measurement data is saved as ASCII file types for use in a spreadsheet or CAE programs. The following three file types are used by the PNA. You can select the content and the format of *.SnP files and *.cti files through the [Define Data Saves](#) dialog box.

***.prn files**

***.SnP (Touchstone)**

***.cti (Citifile)**

*.prn Files

- Read directly into rows and columns by spreadsheet software, such as Microsoft® Excel.
- Contain formatted and corrected stimulus and response data.
- Contain comma-separated list for the current active trace ONLY.
- Are Output only - it cannot be read by the analyzer.

Example:

"S11 Log Mag"

"Frequency (Hz)",	"dB"
3.000000e+005 ,	-3.528682e+001 ,
4.529850e+007 ,	-2.817913e+001 ,
9.029700e+007 ,	-3.216808e+001 ,
1.352955e+008 ,	-3.101017e+001 ,

SnP Format (*.s1p, *.s2p, *.s3p, *.s4p)

This file format is used by CAE programs such as Agilent's Microwave Design System (MDS) and Advanced Design System (ADS).

Note: Frequency Converter Application .S2P files are saved using a different method. See [Using FCA, Save Data.](#)

- SnP data is Output only; it cannot be read by the analyzer.
- SnP data can be saved in various formats. See [Define Data Saves](#)
- The amount of data that is saved depends on the file type that you specify and the amount of data that is available:

File Type	# of Ports	# of S-parameters saved
*.s1p	1	1 S-parameter
*.s2p	2	4 S-parameters
*.s3p	3	9 S-parameters
*.s4p	4	16 S-parameters

SnP data is generally used to gather all S-parameters for a fully corrected measurement. The PNA uses the data that is available on the channel of the active measurement.

- If correction is applied, then valid data is returned for all corrected s-parameters.
- If requesting **less** data then is available, data is returned beginning with the first calibrated ports until your request is fulfilled. For example, if 4-port correction is applied, and you request S3P data, then data is returned for ports 1,2, and 3.
- If correction is NOT applied, the PNA returns as much applicable raw data as possible using S-parameter measurements on the selected channel. Data that is not available is zero-filled. For example, if correction is NOT applied and the active measurement is S11, and an S21 measurement also exists on the channel, then data is returned for the S11 and S21 measurements. Data for S12 and S22 is not available and therefore returned as zeros.
- All valid data is saved using the same format and settings as the active measurement. For example, if the active measurement settings include port extensions, time domain, and smoothing, then all valid data is processed and saved using these same settings.

SnP Data Output

SnP files contain header information, stimulus data, a response data pair for EACH S-parameter measurement. The only difference between S1P, S2P, S3P, and S4P files is the number of S-parameters that are saved.

The following is a sample of **Header information**:

```
!Agilent Technologies,E8362B,US42340026,Q.03.54
!Agilent E8362B: Q.03.54
!Date: Friday, April 25, 2003 13:46:41
!Correction: S11(Full 2 Port SOLT,1,2) S21(Full 2 Port SOLT,1,2) S12(Full 2 Port
SOLT,1,2) S22(Full 2 Port SOLT,1,2)
!S2P File: Measurements:S11,S21,S12,S22:
# Hz S R I R 50
```

Note: Although the following shows Real / Imag pairs, the format could also be LogMag / Phase or LinMag / Phase

*.s1p Files

Each record contains 1 stimulus value and 1 S-parameter (total of 3 values)

Stim Real (Sxx) Imag(Sxx)

*.s2p Files

Each record contains 1 stimulus value and 4 S-parameters (total of 9 values)

Stim Real (S11) Imag(S11) Real(S21) Imag(S21) Real(S12) Imag(S12) Real(S22) Imag(S22)

*.s3p Files

Each record contains 1 stimulus value and 9 S-parameters (total of 19 values)

Stim Real (S11) Imag(S11) Real(S12) Imag(S12) Real(S13) Imag(S13)
Real (S21) Imag(S21) Real(S22) Imag(S22) Real(S23) Imag(S23)
Real (S31) Imag(S31) Real(S32) Imag(S32) Real(S33) Imag(S33)

*.s4p Files

Each record contains 1 stimulus value and 16 S-parameters (total of 33 values)

Stim Real (S11) Imag(S11) Real(S12) Imag(S12) Real(S13) Imag(S13) Real(S14) Imag(S14)
Real (S21) Imag(S21) Real(S22) Imag(S22) Real(S23) Imag(S23) Real(S24) Imag(S24)
Real (S31) Imag(S31) Real(S32) Imag(S32) Real(S33) Imag(S33) Real(S34) Imag(S34)
Real (S41) Imag(S41) Real(S42) Imag(S42) Real(S43) Imag(S43) Real(S44) Imag(S44)

*cti CitiFiles

Citiformat is compatible with the Agilent 8510 Network Analyzer and Agilent's Microwave Design System (MDS). You can do the following using citifiles :

- save the active trace, or all traces. (see [Define Data Saves](#))
- save formatted or unformatted citifile data

Save Formatted data

1. Set the format using [Define Data Saves](#).
2. Click **File** then **Save As**

3. Select **Citifile Formatted Data (*.cti)**

- See Note under [Recalling Citifiles Using the PNA](#)
- On the [data access map](#), Formatted data is taken from location 2 or 4.

Save Unformatted data

1. Click File Save As
2. Select **Citifile Data Data (*.cti)**

On the [data access map](#), Unformatted data is taken from the block just before Format.

Recalling Citifiles Using the PNA

To read citifiles using the PNA, click **File** then **Recall**. Specify **(*.*cti)**

The recalled files are displayed on the PNA using new windows and channels.


- The new window numbers begin with the next available window number.
- New channel numbers begin with channel 9.

When recalling citifiles, an error is displayed if you exceed the PNA [windows and channels limitations](#).


Note: Recalled citifile data is ALWAYS displayed on the PNA using LogMag format, regardless of how the file was stored.

Define Data Saves

How to select Define Data Saves

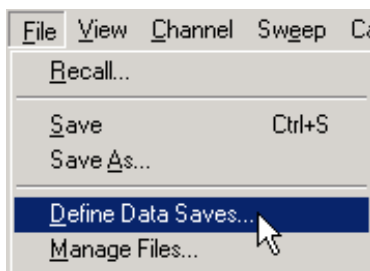

Learn more about using the [front panel interface](#)

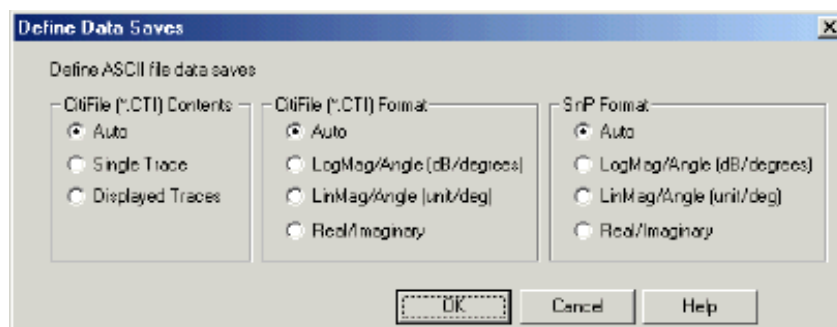

Define Data Saves dialog box help

CitiFile Contents Determines what is saved to a .cti file.

Auto - Saves the active trace. Additional traces are saved if correction is ON and Full 2-port or Full 3-port calibration is performed. For Full 2-port calibration, 4 traces are saved. For Full 3-port calibration, 9 traces are saved.

Single Trace - Saves the active trace in the currently selected window.

Displayed Traces - Saves all displayed data traces

Citifile Formatted Data

Auto - Output is in the currently selected trace format. If other than LogMag, LinMag, or Real/Imag, then output is in Real/Imag.

LogMag, LinMag, Real/Imag - Select output format. All **LogMag** and **LinMag** output is in degrees.

SnP Formatted Data (.s1p, .s2p, .s3p) [Learn more about SnP files.](#)


Auto - Output is in the currently selected trace format. If other than LogMag, LinMag, or Real/Imag, then output is in Real/Imag.

LogMag, LinMag, Real/Imag - Select output format. All **LogMag** and **LinMag** output is in degrees.

Manage Files without a Mouse

The Manage Files dialog box is designed to be used from the front panel. It performs the same function as Windows Explorer, but can be used without the use of a mouse or keyboard.

[Learn more about using the Front-panel interface.](#)

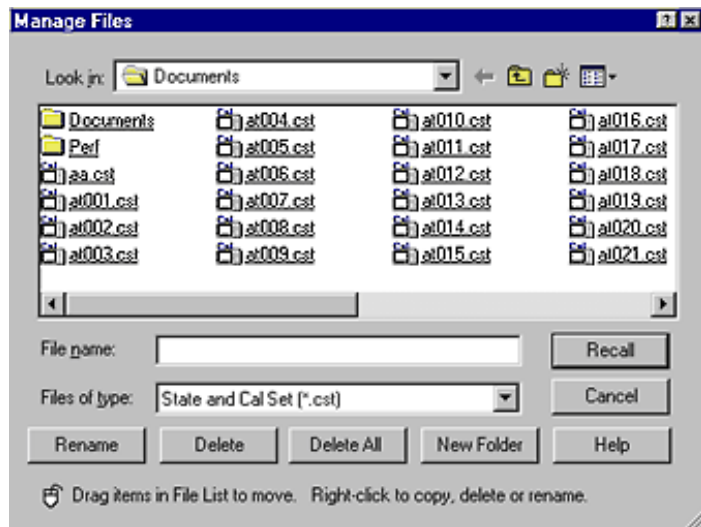

Manage Files dialog box help

Recall Opens a Network Analyzer file already stored in memory.

Rename Renames a file that is selected in the open folder.

Delete Removes a selected file from the open folder.

Delete All Removes all files of the file type selected that appear in the open folder.

New folder Create a new folder and give it a name

Drive Mapping

Drive mapping allows you to share disk drives between the PNA and an external computer. You can either map from the PNA, or from your PC, to the other.

[From the PNA, map to a drive on an External PC](#)

[From an External PC, map to a drive on the PNA](#)

To prepare for Drive Mapping:

1. Both the PC and PNA must be connected to a shared computer network
2. You must know the full computer name of the PC (or analyzer) you are mapping **TO**. [Tell me how](#)
3. Your logon and password on the analyzer must be the same as that on the external PC. You can add your PC logon to the analyzer. [Tell me how](#)

Note: These procedures require a mouse and keyboard. Also, the external PC must have Windows NT 4.0 (or later).

From the Analyzer, map to a drive on the External PC

1. On the external computer desktop, go to **Windows Explorer**. In the listing of drives, right click on the drive you want to share. Click **Sharing**.
2. In the dialog box, select **Shared As**. In the **Share Name** box, use the arrow key or type in a share name for the drive. For example: **C\$**. Click **OK**.
3. On the analyzer desktop, click **Windows Explorer**. From the **Tools** menu, click **Map Network Drive**. (To get to the analyzer desktop, click **View**, then click **Title Bars**)
4. If you would like to connect to your external PC using a different logon, click **Connect using a different Logon**. This logon must be registered on the analyzer and you must be currently logged on the external PC using this logon.



1. In the **Connect as** box, type your logon name.
The logon name and password must be exactly the same on both the external PC and the analyzer.
2. In the **Password** box, type the logon password that you use on the external computer. Click **OK**. The logon name and password must be exactly the same on both the external PC and the analyzer.
5. In the **Folder** box, type `\\(full computer name of analyzer)\share name (from step 2)`. (For example: `\\SLT1234\C$`)
6. Click **Finish**.

From an External PC, map to a drive on the Analyzer

1. On the analyzer desktop, click **Windows Explorer**. Right click on the drive you want to share. Click on **Sharing...**

2. In the dialog box, select **Shared this folder**. In the **Share Name** box, type in a share name for the drive. For example: **C\$**. Click **OK**.
3. On the external PC desktop, click **Windows Explorer**. From the **Tools** menu, click **Map Network Drive**.
4. If the current logon on your PC is different from the current logon on the analyzer, click **Connect using a different Logon** to connect to using the current analyzer logon, .This logon must be registered on the external PC. To see the current logon on either the PC or analyzer, hold **Ctrl - Alt**, and press **Delete**.
 1. In the **Connect as** box, type the logon currently being used by the analyzer.
 2. In the **Password** box, type the logon password that you use on the external computer. Click **OK**
5. In the **Folder** box, type `\\computername (prep1)share name` (from step 2). (For example: `\\SLT1234\C$`)
6. Click **Finish**.

Print a Displayed Measurement

The analyzer allows you to print a displayed measurement to a printer or to a file. The printer can be either a networked or local. Click on a button to learn how to connect to a printer or print a displayed measurement.

[Connecting a Printer](#)

[Printing](#)

Other Outputting Data topics

Connecting a Printer

You can connect your printer to the PNA using three different connector types:

- [Parallel connector](#)
- [Serial connector](#)
- [USB](#)

Note: Early PNAs have a Centronics connector for connecting a printer. An adapter (36-pin male - 1284-C - to 25-pin female) was shipped with those PNAs to allow connection with a standard parallel printer cable.

CAUTION: Do NOT connect your printer to the 25-pin female port labeled **Ext. Test Set Interface**. Voltage levels of signal lines may damage the printer's I/O.

To Add a Printer

Note: If you try to print from the PNA application and the **Add Printer Wizard** appears, click **Cancel** and add the printer using the following procedure.

1. From the PNA application, click **View** then click **Minimize Application**
2. On the Windows taskbar, click **Start**, point to **Settings**, then click **Printers**.
3. Double-click **Add Printer**.
4. Follow the instructions in the **Add Printer** Wizard.

For more information, refer to Microsoft Windows Help or your printer documentation.

Printing


[Print a Hardcopy](#)

[Print Options](#)

[Print to File](#)


The measurement information on the screen can be printed to any local or networked printer that is connected to the analyzer. The amount of measurement information printed is selected by the print options settings.

The graphic below shows an example of how a screen-capture image appears when printed. The [print options](#) settings allows you to customize the printed form of the measurement information.

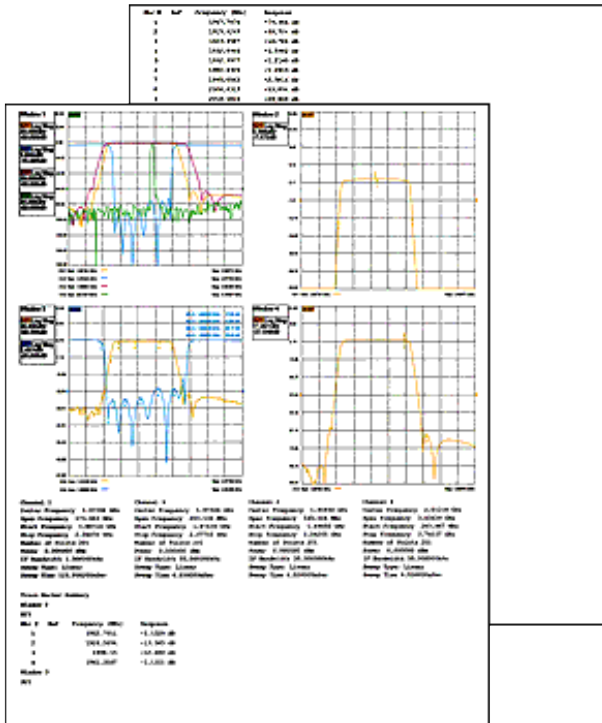

How to Print a Hardcopy

Use one of the following methods

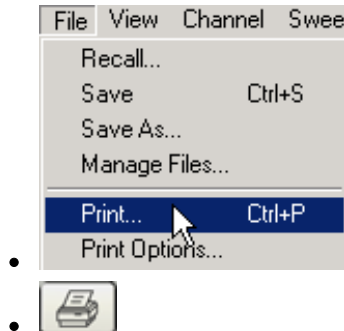


Learn more about using the [front panel interface](#)

Note: For information on the choices in the Print dialog box, see Windows 2000 Help.


Print Options

The Print Options Dialog Box allows flexibility in the appearance that measurement data is printed. After selecting the options, click **Print...** to obtain a hard-copy.

How to select Print Options

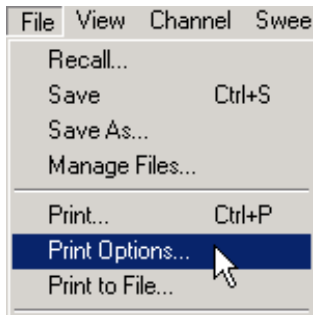

Learn more about using the [front panel interface](#)

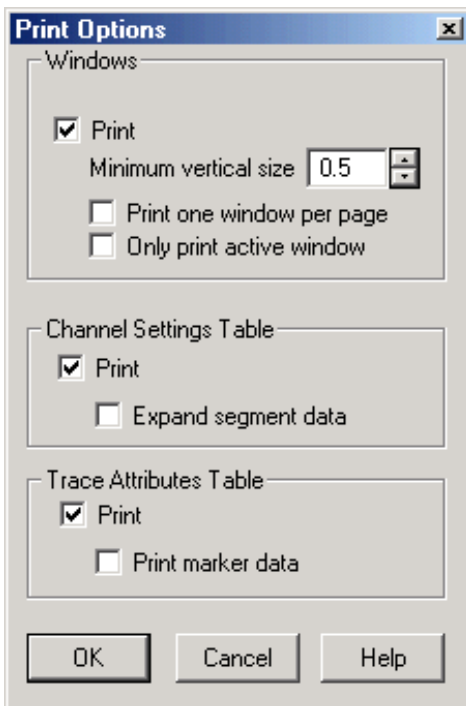

Print Options dialog box help

Windows

Print Check to print measurement windows.

Minimum vertical size Adjust to change the amount of a page that the measurement window fills. The adjustment range is from .4 to 1.0 of a page.

Print one window per page Check to print one window per page. Clear to print all selected windows without a forced page break.

Only print active window Check to print only the active window. Clear to print all windows.

Channel Settings Table

Print Check to print the channel settings table.

Expand segment data Check to print segment data. The amount of data depends on how much the sweep is segmented.

Trace Attributes Table

Print Check to print the Trace Attributes Table. The Trace Attributes are measurement type, correction factors ON or OFF, smoothing, options, and marker details. The Trace Attributes are listed by Trace ID# for each window.

Each Trace ID# can have multiple entries depending on the number of markers associated with the trace. The marker details are marker number, position and response. If there are multiple markers on a trace, the trace attributes are only shown for the first marker. However, the trace attributes for the first marker apply to all other markers on that trace.

The options column can have one or more options. **D** for Delay, **M** for Marker, **G** for Gating. Multiple options selected would appear as follows: DMG.

Print marker data Check to print all marker data. The amount of data depends on how many markers are created.

Print to a File


The analyzer can save a screen-capture image in any of the following formats:

- **.png** (preferred format)
- **.bmp** (bitmap)
- **.jpg**

The analyzer automatically saves the file to the current path. If not previously defined, the analyzer automatically selects the default path C:\Program Files\Agilent\Network Analyzer\Documents\

A .bmp file, like a .prn file, can be imported into software applications such as Microsoft Excel, Word, or Paint to display a screen-capture image.

How to Print to a File

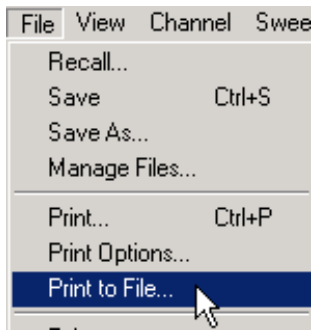

Learn more about using the [front panel interface](#)

See [Save and Recall files](#) for more information.

Network Analyzer Basics

This multimedia presentation is intended to run on the PNA.

[Click to proceed with Network Analyzer Basics.](#)

To view this presentation on an external PC, copy the all of the files from the PNA C:\WINNT\Help\NABasics to the same location on your PC's hard drive. The total file size is approximately 100MB.

Connector Care

Proper connector care is critical for accurate and repeatable measurements. The following information will help you preserve the precision and extend the life of your connectors - saving both time and money.

[Connector Care Quick Reference Guide](#)

[Connector Cleaning Supplies](#)

[Safety Reminders](#)

[About Connectors](#)

[Gaging Fundamentals](#)

[Connector Care Procedures](#)

Connector Care Quick Reference Guide

Handling and Storing Connectors	
Do	Do Not
Keep connectors clean Protect connectors with plastic end caps Keep connector temperature same as analyzer	Touch mating-plane surfaces Set connectors contact-end down Store connectors loose in box or drawer
Visual Inspection	
Do	Do Not
Inspect connectors with magnifying glass. Look for metal debris, deep scratches or dents	Use a connector with a bent or broken center conductor Use a connector with deformed threads
Cleaning Connectors	
Do	Do Not
Clean surfaces first with clean, dry compressed air Use lint-free swab or brush Use minimum amount of alcohol Clean outer conductor mating surface and threads	Use high pressure air (>60 psi) Use any abrasives Allow alcohol into connector support beads Apply lateral force to center conductor
Gaging Connectors	
Do	Do Not

Inspect and clean gage, gage master and device tested Use correct torque wrench zero gage before use Use multiple measurements and keep record of readings	Use an out of specification connector Hold connector gage by the dial
Making Connections	
Do	Do Not
Align connectors first Rotate only the connector nut Use correct torque wrench	Cross thread the connection Twist connector body to make connection Mate different connector types

Connector Care and Cleaning Supplies

Listed below are products commonly used for connector cleaning. To order these and other connector care products, see [Analyzer Accessories](#).

Description	Agilent P/N
Lint-Free Swabs, small 100 ct.	9301-1243
IPA 99.5% alcohol, 30 ml bottle	8500-5344
Compressed Air, 235 ml can	8500-6659

Safety Reminders

When cleaning connectors:

- Always use protective eyewear when using compressed air or nitrogen.
- Keep isopropyl alcohol away from heat, sparks and flame. Use with adequate ventilation. Avoid contact with eyes, skin and clothing.
- Avoid electrostatic discharge (ESD). Wear a grounded wrist strap (having a 1 M Ω series resistor) when cleaning device, cable or test port connectors.

About Connectors

[Connector Service Life](#)

[Connector Grades and Performance](#)

[Adapters as Connector Savers](#)

[Connector Mating Plane Surfaces](#)

Connector Service Life

Even though calibration standards, cables, and test set connectors are designed and manufactured to the highest standards, all connectors have a limited service life. This means that connectors can become defective due to wear during normal use. For best results, all connectors should be inspected and maintained to maximize their service life.

Visual Inspection should be performed each time a connection is made. Metal particles from connector threads often find their way onto the mating surface when a connection is made or disconnected. See [Inspection](#) procedure.

Cleaning the dirt and contamination from the connector mating plane surfaces and threads can extend the service life of the connector and improve the quality of your calibration and measurements. See [Cleaning](#) procedure.

Gaging connectors not only provides assurance of proper mechanical tolerances, and thus connector performance, but also indicate situations where the potential for damage to another connector may exist. See [Gaging](#) procedure.

Proper connector care and connection techniques yield:

- Longer Service Life
- Higher Performance
- Better Repeatability

Connector Grades and Performance

The three connector grades (levels of quality) for the popular connector families are listed below. Some specialized types may not have all three grades.

- **Production** grade connectors are the lowest grade and the least expensive. It is the connector grade most commonly used on the typical device under test (DUT). It has the lowest performance of all connectors due to its loose tolerances. This means that production grade connectors should always be carefully inspected before making a connection to the analyzer. Some production grade connectors are not intended to mate with metrology grade connectors.
- **Instrument** grade is the middle grade of connectors. It is mainly used in and with test instruments, most cables and adapters, and some calibration standards. It provides long life with good performance and tighter tolerances. It may have a dielectric supported interface and therefore may not exhibit the excellent match of a metrology grade connector.
- **Metrology** grade connectors have the highest performance and the highest cost of all connector grades. This grade is used on calibration standards, verification standards, and precision adapters. Because it is a high precision connector, it can withstand many connections and disconnections and, thus, has the longest life of all connector grades. This connector grade has the closest material and geometric specifications. Pin diameter and pin depth are very closely specified. Metrology grade uses an air dielectric interface and a slotless female contact which provide the highest performance and traceability.

Note: In general, Metrology grade connectors should not be mated with Production grade connectors.

Adapters as Connector Savers


Make sure to use a high quality (Instrument grade or better) adapter when adapting a different connector type to the analyzer test ports. It is a good idea to use an adapter even when the device under test is the same connector type as the analyzer test ports. In both cases, it will help extend service life, and protect the test ports from damage and costly repair.

The adapter must be fully inspected before connecting it to the analyzer test port and inspected and cleaned frequently thereafter. Because calibration standards are connected to the adapter, the adapter should be the highest quality to provide acceptable RF performance and minimize the effects of mismatch.

Connector Mating Plane Surfaces

An important concept in RF and microwave measurements is the reference plane. For a network analyzer, this is


the surface that all measurements are referenced to. At calibration, the reference plane is defined as the plane where the mating plane surfaces of the measurement port and the calibration standards meet. Good connections (and calibrations) depend on perfectly flat contact between connectors at all points on the mating plane surfaces (as shown in the following graphic).

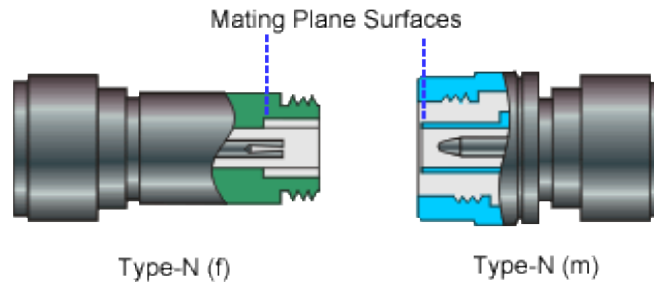

Gaging Fundamentals

Connector gages are important tools used to measure center conductor pin depth in connectors. Connector pin depth, measured in terms of recession or protrusion, is generally the distance between the mating plane and the end of the center conductor, or the shoulder of the center conductor for a stepped male pin.


Typical Connector Gage

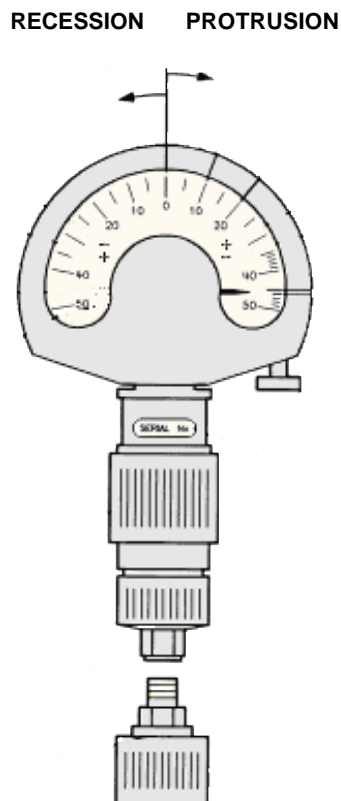

Recession and Protrusion

Pin depth is negative (recession) if the center conductor is recessed below the outer conductor mating plane, usually referred to as the "reference plane". Pin depth is positive (protrusion) if the center conductor projects forward from the connector reference plane.

Pin Depth

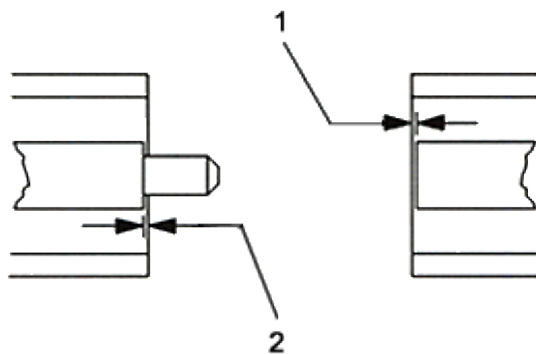

1. Recession of female contact
2. Recession of male pin shoulder

Difference with Type-N Connectors

Type-N connectors have the mating plane of the center conductors offset from the connector reference plane. In this case the zero setting "gage masters" generally offset the nominal distance between the center conductor mating plane and the connector reference plane.

When to Gage Connectors

- Before using a connector or adapter the first time.
- When visual inspection or electrical performance suggests the connector interface may be out of range.
- After every 100 connections, depending on use.

Connector Gage Accuracy

Connector gages (those included with calibration and verification kits), are capable of performing coarse measurements only. This is due to the repeatability uncertainties associated with the measurement. It is important to recognize that test port connectors and calibration standards have mechanical specifications that are extremely precise. Only special gaging processes and electrical testing (performed in a calibration lab) can accurately verify the mechanical characteristics of these devices. The pin depth specifications in the Agilent calibration kit manuals provide a compromise between the pin depth accuracy required, and the accuracy of the gages. The gages shipped with calibration and verification kits allow you to measure connector pin depth and avoid damage from out-of-specification connectors.

Note: Before gaging any connector, the mechanical specifications provided with that connector or device should be checked.

To Gage Connectors

1. Wear a grounded wrist strap (having a 1 M Ω series resistor).
2. Select proper gage for device under test (DUT).
3. Inspect and clean gage, gage master, and DUT.
4. Zero the connector gage.
 - a. While holding gage by the barrel, carefully connect gage master to gage. Finger-tighten connector nut only.
 - b. Use proper torque wrench to make final connection. If needed, use additional wrench to prevent gage

master (body) from turning. Gently tap the barrel to settle the gage.

c. The gage pointer should line up exactly with the zero mark on gage. If not, adjust "zero set" knob until gage pointer reads zero. On gages having a dial lock screw and a movable dial, loosen the dial lock screw and move the dial until the gage pointer reads zero. Gages should be zeroed before each set of measurements to make sure zero setting has not changed.

d. Remove gage master.

5. Gage the device under test.

a. While holding gage by the barrel, carefully connect DUT to gage. Finger-tighten connector nut only.

b. Use proper torque wrench to make final connection and, if needed, use additional wrench to prevent DUT (body) from turning. Gently tap the barrel to settle the gage.

c. Read gage indicator dial for recession or protrusion and compare reading with device specifications.

Caution: If the gage indicates excessive protrusion or recession, the connector should be marked for disposal or sent out for repair.

6. For maximum accuracy, measure the device a minimum of three times and take an average of the readings. After each measurement, rotate the gage a quarter-turn to reduce measurement variations.

7. If there is doubt about measurement accuracy, be sure the temperatures of the parts have stabilized. Then perform the cleaning, zeroing, and measuring procedure again.

Connector Care Procedures

Inspecting Connectors

Cleaning Connectors

Making Connections

Using a Torque Wrench

Handling and Storing Connectors

To Inspect Connectors

Wear a grounded wrist strap (having a 1 M Ω series resistor).


Use a magnifying glass ($\geq 10X$) and inspect connector for the following:

- Badly worn plating or deep scratches
- Deformed threads
- Metal particles on threads and mating plane surfaces
- Bent, broken, or mis-aligned center conductors
- Poor connector nut rotation


Caution: A damaged or out-of-specification device can destroy a good connector attached to it even on the first connection. Any connector with an obvious defect should be marked for disposal or sent out for repair.

To Clean Connectors

1. Wear a grounded wrist strap (having a 1 M Ω series resistor).
2. Use clean, low-pressure air to remove loose particles from mating plane surfaces and threads. Inspect connector thoroughly. If additional cleaning is required, continue with the following steps.

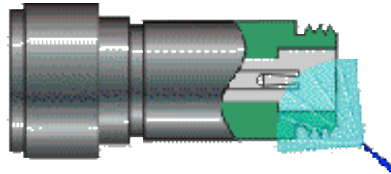

3. Moisten—do not saturate—a lint-free swab with isopropyl alcohol. See [Cleaning Supplies](#) for recommended type.
4. Clean contamination and debris from mating plane surfaces and threads. When cleaning interior surfaces, avoid exerting pressure on center conductor and keep swab fibers from getting trapped in the female center conductor.

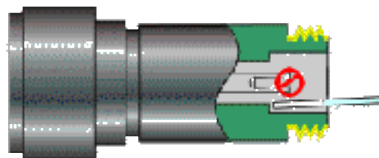

5. Let alcohol evaporate—then use compressed air to blow surfaces clean.
6. Inspect connector. Make sure no particles or residue remains.
7. If defects are still visible after cleaning, the connector itself may be damaged and should not be used. Determine the cause of damage before making further connections.


To Make Connections

1. Wear a grounded wrist strap (having a 1 M Ω series resistor).
2. Inspect, clean, and gage connectors. All connectors must be undamaged, clean, and within mechanical specification.
3. Carefully align center axis of both devices. The center conductor pin—from the male connector—must slip concentrically into the contact finger of the female connector.




4. Carefully push the connectors straight together so they can engage smoothly. Rotate the connector nut (not

the device itself) until finger-tight, being careful not to cross the threads.

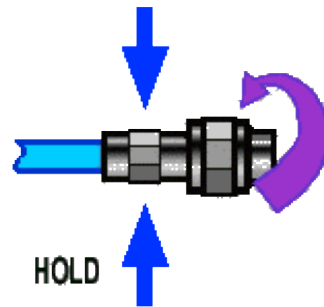

5. Use a torque wrench to make final connection. Tighten until the "break" point of the torque wrench is reached. Do **not** push beyond initial break point. Use additional wrench, if needed, to prevent device body from turning.

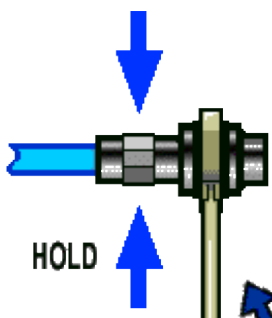


To Separate a Connection

1. Support the devices to avoid any twisting, rocking or bending force on either connector.
2. Use an open-end wrench to prevent the device body from turning.
3. Use another open-end wrench to loosen the connector nut.
4. Complete the disconnection by hand, turning only the connector nut.
5. Pull the connectors straight apart.


To Use a Torque Wrench

1. Make sure torque wrench is set to the correct torque setting.
2. Position torque wrench and a second wrench (to hold device or cable) within 90° of each other before applying force. Make sure to support the devices to avoid putting stress on the connectors.

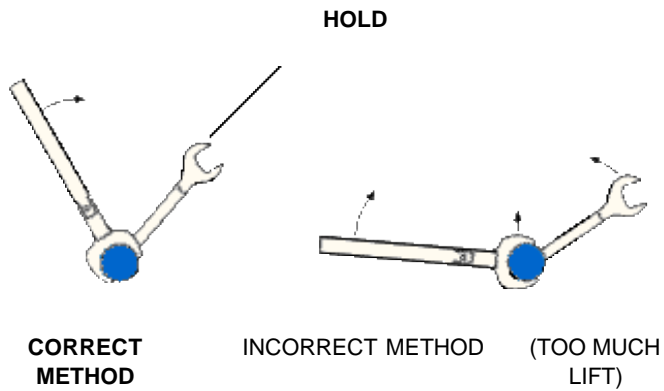

3. Hold torque wrench lightly at the end of handle—then apply force perpendicular to the torque wrench handle. Tighten until the "break" point of the torque wrench is reached. Do **not** push beyond initial break point.

TORQUING DIRECTION

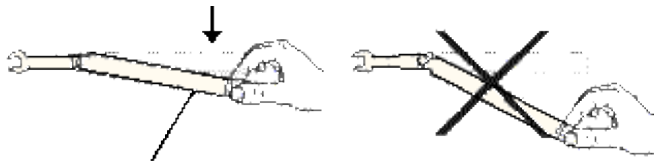

STOP WHEN HANDLE BEGINS TO YIELD

To Handle and Store Connectors


- Install protective end caps when connectors are not in use.
- Never store connectors, airlines, or calibration standards loose in a box. This is a common cause of connector damage.
- Keep connector temperature the same as analyzer. Holding the connector in your hand or cleaning connector with compressed air can significantly change the temperature. Wait for connector temperature to stabilize before using in calibration or measurements.
- Do not touch mating plane surfaces. Natural skin oils and microscopic particles of dirt are difficult to remove from these surfaces.
- Do not set connectors contact-end down on a hard surface. The plating and mating plane surfaces can be damaged if the interface comes in contact with any hard surface.
- Wear a grounded wrist strap and work on a grounded, conductive table mat. This helps protect the analyzer and devices from electrostatic discharge (ESD).

Electrostatic Discharge (ESD) Protection

Protection against electrostatic discharge (ESD) is essential while removing or connecting cables to the network analyzer. Static electricity can build up on your body and can easily damage sensitive internal circuit elements when discharged. Static discharges too small to be felt can cause permanent damage. To prevent damage to the instrument:

- Always have a grounded, conductive table mat in front of your test equipment.
- Always wear a grounded wrist strap, connected to a grounded conductive table mat, having a 1 MO resistor in series with it, when making test setup connections.
- Always wear a heel strap when working in an area with a conductive floor. If you are uncertain about the conductivity of your floor, wear a heel strap.
- Always ground yourself before you clean, inspect, or make a connection to a static-sensitive device or test port. You can, for example, grasp the grounded outer shell of the test port or cable connector briefly.
- Always ground the center conductor of a test cable before making a connection to the analyzer test port or other static-sensitive device. This can be done as follows:
 1. Connect a short (from your calibration kit) to one end of the cable to short the center conductor to the outer conductor.
 2. While wearing a grounded wrist strap, grasp the outer shell of the cable connector.
 3. Connect the other end of the cable to the test port and remove the short from the cable.

The following graphic shows a typical ESD protection setup using a grounded mat and wrist strap. Refer to [Analyzer Accessories](#) for part numbers.

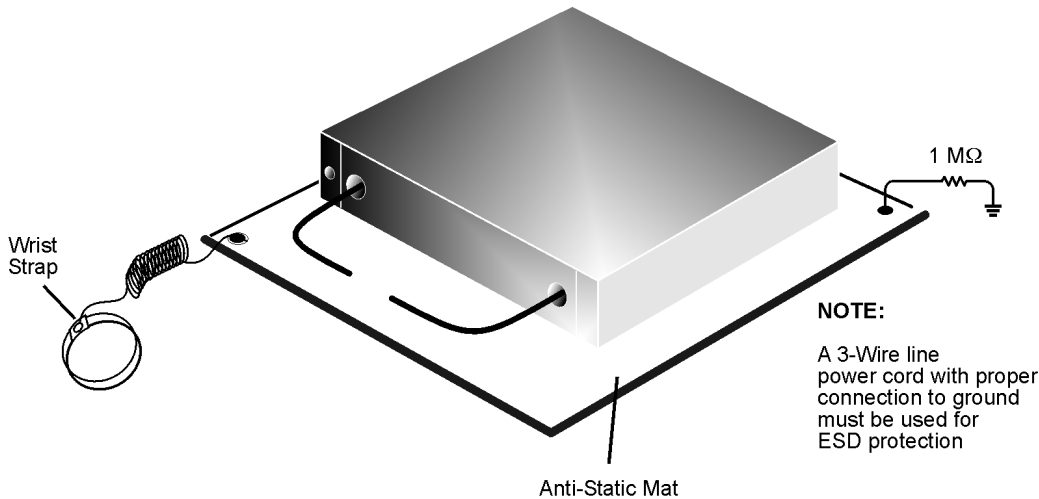

esd_setup

Impedance Matching Model

Impedance matching is a procedure used in circuit design to match unequal source and load impedances, thereby optimizing the power delivered to the load from the source. Impedance matching is accomplished by inserting matching networks into a circuit between the source and the load.

[Introduction to the Model](#)

[Impedance Matching Model](#)

[Description of Exercises](#)

[Smith Chart Circuit Elements Paths](#)



[Forbidden Regions of the Smith Chart](#)

Other Tutorials topics


Introduction

In this model, Smith Charts are used to visualize the interactive process of impedance matching to optimize transmitted power in simple circuits. Simple series/shunt, inductance/capacitance matching networks are used, and you can interactively adjust the values of corresponding L and C components. Adjusting the matching network components changes the reflectance of the overall circuit. The reflectance of each part of the circuit is indicated on the Smith Chart as a red ● or blue ● ball.

As you adjust the sliders and modify the component values, the model calculates new values for the circuit reflectance and moves the red ● and blue ● balls on the Smith Chart. The goal of each exercise is to move the reflectance point from the center of the Smith Chart, which represents either the load or source, into the


appropriate  red and  blue rings which represent the desired matching condition. You can select three different impedance matching problems of increasing difficulty by clicking on one of the three labeled tabs.

Impedance Matching Model

 maximize this window for optimum viewing. [Click](#) if the Impedance model is not visible.


Description of Exercises

L-C Matching Network

The first exercise lets you use the Smith Chart to perform basic impedance matching between a resistive source and a resistive load. A simple series-inductance shunt-capacitance network is used to match the 50 ohm source to the 300 ohm load. The source reflectance of the circuit looking from the load toward the source is represented by the red ball ●, while the 300 ohm load is indicated by the stationary  red ring.


The objective of the exercise is to interactively match these two impedances by adjusting the L and C sliders. The model will provide graphical feedback by moving the red ball indicating circuit reflectance on the Smith Chart. Adjust the series L and shunt C sliders to move the reflectance point ● from the center of the Smith Chart to the matching impedance position inside the red ring. You can study the [Smith Chart Circuit Element Paths](#) below for hints on how different circuit elements change circuit reflectance on the Smith Chart.

Transistor Amplifier-I

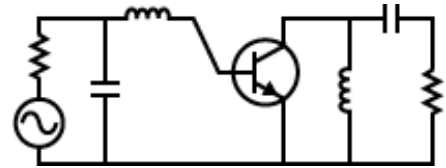

The second exercise provides the impedance matching experience of optimizing the transducer power gain of a transistor amplifier. Matching the 50 ohm source to the input reflectance of the transistor, s^{*11} , and matching the 50 ohm load to the output reflectance of the transistor, s^{*22} , optimizes the power delivered from the source, through the transistor, to the load. You are required to match both the input red ball ● and output blue ball ● of the transistor separately. Adjust the component values to move both reflectance points to their proper positions within the red ○ and blue ○ rings.

Transistor Amplifier-II

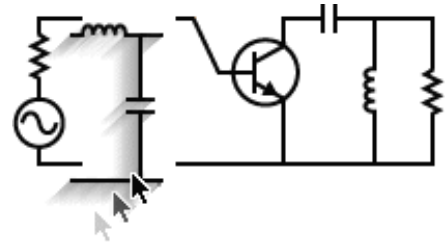


The third part of the interactive impedance matching model is a collection of exercises involving a modular circuit. You begin by constructing a circuit with either one or two modular drag-and-drop matching network components. Once the matching networks have been added to the circuit, the sliders will become active and allow you to adjust the component values. Then you will engage in impedance matching for the circuit you have just created! There are 8 different circuits you can construct and there are 5 different value pairs for s^{*11} and s^{*22} on the Smith Chart, altogether 40 impedance matching exercises. **You will find that not all matching networks will work!** For some of the circuits you will be able to construct, you will not be able to position the red ball ● within the red ring or the blue ● ball within the blue ring. To determine in advance which matching networks will work, take a close look at the [Forbidden Regions of the Smith Chart](#) below. There are 5 different location pairs for s^{*11} and s^{*22} corresponding to different frequencies that can be matched. Use the frequency indicator to select an operating frequency, and then drag-and-drop appropriate matching networks into the circuit and adjust the component values to move both reflectance points to their proper positions within the red ○ and blue rings.

Smith Chart Circuit Elements Paths

The graphs below demonstrate how the various shunt and series L and C components change the circuit reflectance on the Smith Chart. Assuming the given component is the last component in the matching network, the circuit reflectance will move as indicated along constant resistance or constant conductance circles.

You can think of impedance matching using the Smith Chart as driving a car to a specific destination in Smith Town - a city where none of the streets are straight! By adjusting circuit components in appropriate order, we can constrain the circuit reflectance to paths along constant resistance or constant conductance circles. Just like road signs can direct a car along the circular streets of Smith Town, so can we reach the matching impedance condition in a straightforward and deterministic way.




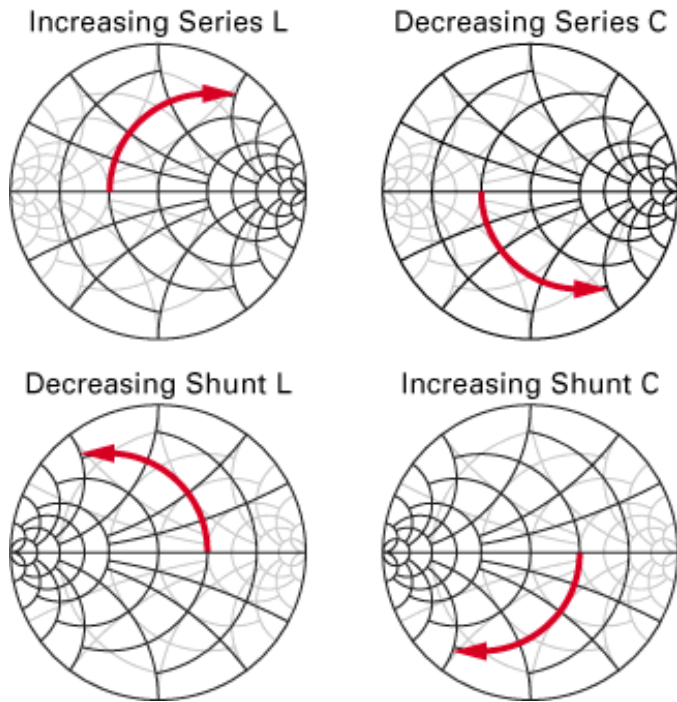


Forbidden Regions of the Smith Chart

For a given load reflectance, only certain L-C matching networks will be capable of transforming the source impedance to the load impedance. In fact, for any load reflectance, exactly two of the four possible L-C matching networks in the Transistor Amplifier-II model above will be able to do the matching job. But which two?

The charts below can be used to determine which matching networks will work in a given load situation. If the load reflectance lies within the forbidden region of the Smith Chart for the indicated matching network, then that network cannot perform the required matching operation. **You cannot drive your car into the forbidden neighborhoods of Smith Town! They are unpaved!**

Use these charts to determine which matching network should be used. First, visually locate the position of the load reflectance from the Transistor Amplifier-II model above on each of the four color Smith Charts below. Then, eliminate the two networks whose forbidden regions overlap the reflectance point, and use one of the remaining two networks to perform the impedance match.

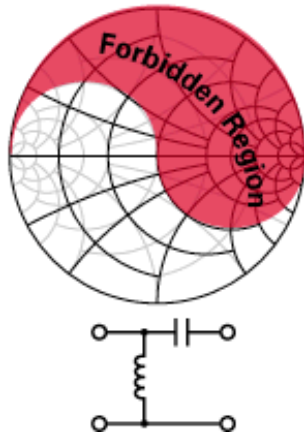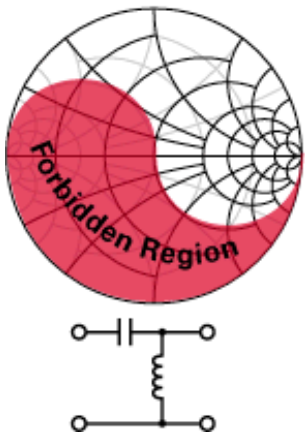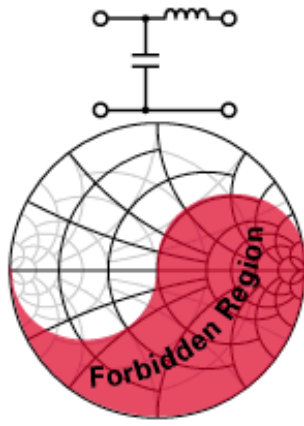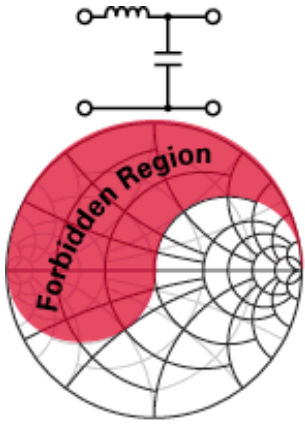

Reflected Waves Along a Transmission line

When a sine wave from an RF signal generator is placed on a transmission line, the signal propagates toward the load. This signal, shown here in yellow, appears as a set of rotating vectors, one at each point on the transmission line.

Maximize this window for optimum viewing. **Click** if the applet is not visible.

In our example, the transmission line has a characteristic impedance of 50 ohms. If we choose a load of 50 ohms, then the amplitude of the signal will not vary with position along the line. Only the phase will vary along the line, as shown by the rotating vectors in yellow.

If the load impedance does not perfectly match the characteristic impedance of the line, there will be a reflected signal that propagates toward the source. At any point along the transmission line, that signal also appears to be a constant voltage whose phase is dependent upon physical position along the line.

The voltage seen at one particular point on the line will be the vector sum of the transmitted and reflected sinusoids. We can demonstrate this by looking at two examples.

Example 1: Perfect Match: 50 Ohms

Set the terminating resistor to 50 ohms by using the "down arrow" dialog box. Notice there is no reflection. We have a perfect match. Each rotating vector has a normalized amplitude of 1. If we were to observe the waveform at any point with a perfect measuring instrument, we would see equal sine wave amplitudes anywhere along the transmission line. The signal amplitudes are indicated by the green line.

Example 2: Mismatched Load: 200 Ohms

Now let's intentionally create a mismatched load. Set the terminating resistor to 200 ohms by using the down arrow. Hit the PLAY button and notice the change in the reflected waveform. If it were possible to measure just the reflected wave, we would see that its amplitude does not vary with position along the line. The only difference between the reflected (blue) signal, say at point z6 and point z4, is the phase.

But the amplitude of the resultant waveform, indicated by the standing wave (green), is not constant along the entire line because the transmitted and reflected signals (yellow and blue) combine. Since the phase between the transmitted and reflected signals varies with position along the line, the vector sums will be different, creating what's called a "standing wave".

With the load impedance at 200 ohms, a measuring device placed at point z6 would show a sine wave of constant amplitude. The sine wave at point z4 would also be of constant amplitude, but its amplitude would differ from that of the signal at point z6. And the two would be out of phase with each other. Again, the difference is shown by the green line, which indicates the amplitude at that point on the transmission line.

The impedance along the line also changes, as shown by the points labeled z1 through z7.

Reflection Measurements

Reflection measurements are an important part of network analysis.

What are Reflection Measurements?

Why Make Reflection Measurements?

Expressing Reflected Waves

Return Loss

VSWR

Reflection Coefficient


Impedance

Summary of Expressions

[See other Tutorials](#)

What are Reflection Measurements?

To understand reflection measurements, it is helpful to think of traveling waves along a transmission line in terms of a lightwave analogy. We can imagine incident light striking some optical component like a clear lens. Some of the light is reflected off the surface of the lens, but most of the light continues on through the lens. If the lens had mirrored surfaces, then most of the light would be reflected and little or none would be transmitted.

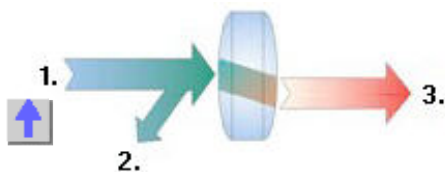

1. Incident 2. Reflected 3. Transmitted

With RF energy, reflections occur when the impedance of two mated devices are not the same. A reflection measurement is the ratio of the reflected signal to the incident signal. Network analyzers measure the incident wave with the R (for reference) channel and the reflected wave with the A channel. Therefore, reflection is often shown as the ratio of A over R (A/R). We can completely quantify the reflection characteristics of our device under test (DUT) with the amplitude and phase information available at both the A and R channel. In S-parameter terminology, S_{11} is a reflection measurement of port1 of the device (the input port); S_{22} is a reflection measurement of the port 2 (the output port)

Why Make Reflection Measurements?


One reason we make reflection measurements to assure efficient transfer of RF power. We do this because:

1. RF energy is not cheap. When energy is reflected, that means less energy is transmitted to where it is

intended to go.

2. If the reflected energy is large, it can damage components, like amplifiers.

For example, in the following graphic, the radio station on the left is not operating at peak efficiency. The amplifier impedance is not the same as the transmission line, and the transmission line impedance is not the same as the antenna. Both of these conditions cause high reflected power. This condition results in less transmitted power, and the high reflected power could damage the amplifier.

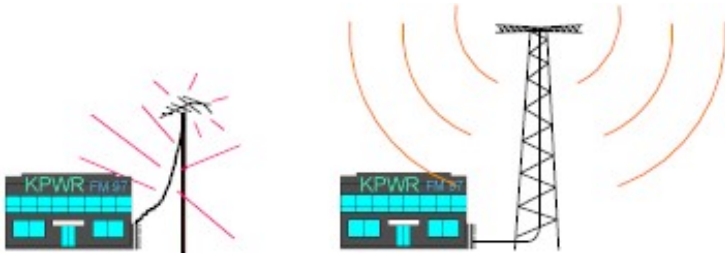

The radio station on the right installed properly "matched" transmission line and antenna. Very little of the transmitted signal is reflected, resulting in increased broadcast power, more listeners, more advertising revenue, and more profit. The amplifier, transmission, and antenna all need to be measured to ensure that reflected power is minimized.

Expressing Reflected Waves

After making a reflection measurement, the reflection data can be expressed in a number of ways, depending on what you are trying to learn. The various expressions are all calculated by the analyzer from the same reflection measurement data. Each method of expressing reflection data can be graphically displayed in one or more formats. For more information, see display formats.

Return Loss

The easiest way to convey reflection data is return loss. Return loss is expressed in dB, and is a scalar (amplitude only) quantity. Return loss can be thought of as the absolute value or dB that the reflected signal is below the incident signal. Return loss varies between infinity for a perfect impedance match and 0 dB for an open or short circuit, or a lossless reactance. For example, using the log magnitude format on the analyzer, the measured reflection value on the screen may be -18dB. The minus sign is ignored when expressing return loss, so the component is said to have 18dB of return loss.

VSWR

Two waves traveling in opposite directions on the same transmission line cause a "standing wave". This condition can be measured in terms of the voltage standing wave ratio (VSWR or SWR for short). VSWR is defined as the maximum reflected voltage over the minimum reflected voltage at a given frequency. VSWR is a scalar (amplitude only) quantity. VSWR varies between one for a perfect match, and infinity for an open or short circuit or lossless reactance.

Reflection Coefficient

Another way of expressing reflection measurements is reflection coefficient gamma (Γ). Gamma includes both magnitude and phase.

The magnitude portion of gamma is called rho (ρ). Reflection coefficient is the ratio of the reflected signal voltage to the incident signal voltage. The range of possible values for ρ is between zero and one. A transmission line terminated in its characteristic impedance will have all energy transferred to the load; zero energy will be reflected and $\rho = 0$. When a transmission line terminated in a short or open circuit, all energy is reflected and $\rho = 1$. The value of rho is unitless.


Now for the phase information. At high frequencies, where the wavelength of the signal is smaller than the length of conductors, reflections are best thought of as waves moving in the opposite direction of the incident waves. The incident and reflected waves combine to produce a single "standing" wave with voltage that varies with position

along the transmission line.


When a transmission line is terminated in its characteristic impedance (Z_0) there is no reflected signal. All of the incident signal is transferred to the load, as shown in the following graphic. There is energy flowing in one direction along the transmission line.




When a transmission line is terminated in a short circuit termination, all of the energy is reflected back to the source. The reflected wave is equal in magnitude to the incident wave ($\rho = 1$). The voltage across any short circuit is zero volts. Therefore, the voltage of the reflected wave will be 180 degrees out of phase with the incident wave, canceling the voltage at the load.

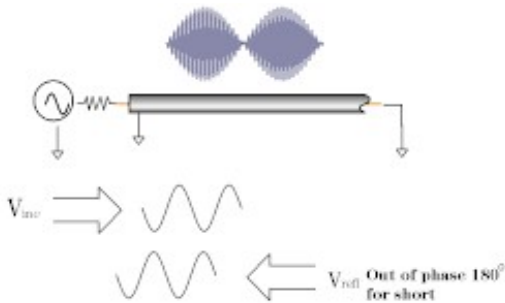

When a transmission line is terminated in an open circuit termination, all of the energy is reflected back to the source. The reflected wave is equal in magnitude to the incident wave ($\rho = 1$). However, no current can flow in an open circuit. Therefore, the voltage of the reflected wave will be in phase with the voltage of the incident wave.

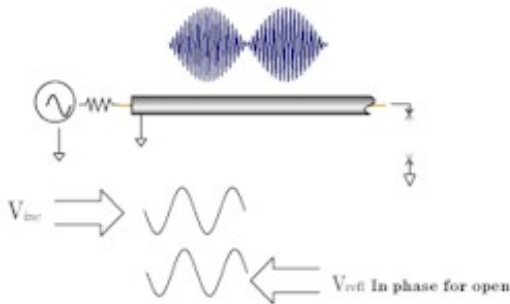

When a transmission line is terminated in a 25 ohm resistor, some but not all of the incident energy will be absorbed, and some will be reflected back towards the source. The reflected wave will have an amplitude 1/3 that of the incident wave and the voltage of the two waves will be out of phase by 180 degrees at the load. The phase relationship will change as a function of distance along the transmission line from the load. The valleys of the standing wave pattern will no longer go to zero, and the peaks will be less than that of the open / short circuit.

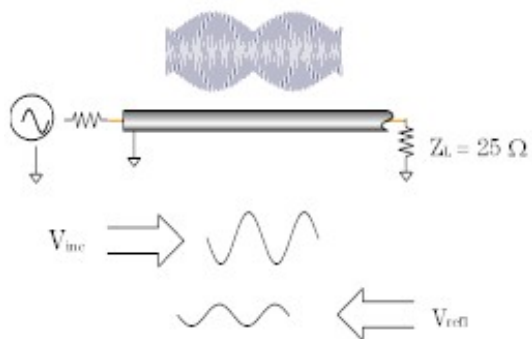


For more information, see [Phase Measurements](#).

Impedance

Impedance is another way of expressing reflection data. For more information on Impedance, see [Smith Charts](#).

Summary of the Expressions of Reflection Measurements:

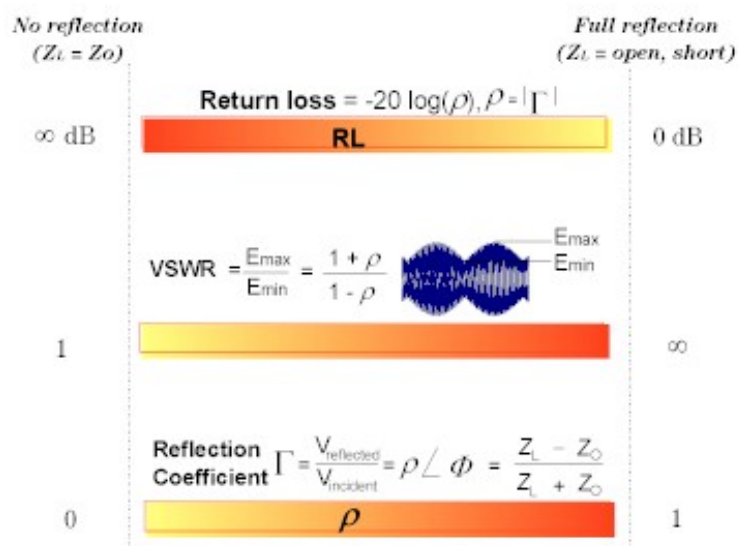

Phase Measurements

Knowledge of both magnitude and phase characteristics is needed for successful higher-level component integration.

[What are Phase Measurements?](#)

[Why Measure Phase?](#)

[Using the Analyzer's Phase Format](#)


[Types of Phase Measurements](#)

[See other Tutorials](#)

What are Phase Measurements?


Phase measurements are made using S-parameters, just like amplitude measurements. A phase measurement is a relative (ratio) measurement and not an absolute measurement. Phase measurements compare the phase of the signal going into a device (the incident signal) to the phase of the device's response signal. The response signal can be either reflected or transmitted. Assuming an accurate calibration has been performed, the difference in phase between the two signals (known as phase shift) is a result of the electrical characteristics of the device under test.

The following graphic shows the phase shift (in time or degrees) between an incident signal and a transmitted signal (as might be seen on an oscilloscope display).

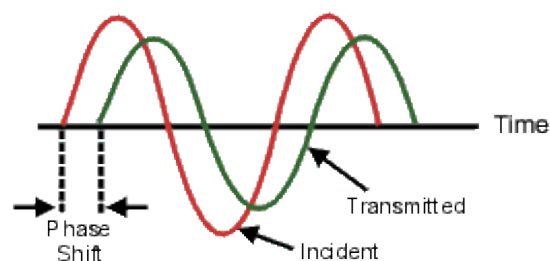

Why Measure Phase?

Measuring phase is a critical element of network analysis. The following graphic lists five reasons for measuring both magnitude and phase.

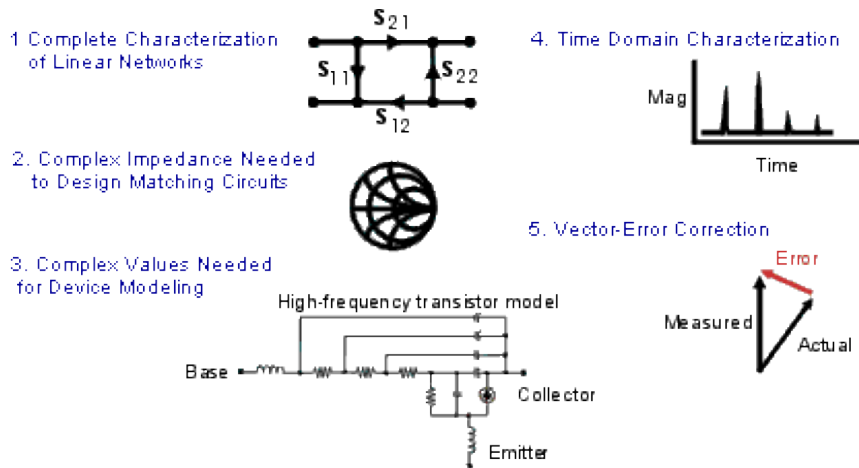


When used in communications systems to pass signals, components or circuits must not cause excessive signal distortion. This distortion can be:

- Linear, where flat magnitude and linear phase shift versus frequency is not maintained over the bandwidth of interest.
- Nonlinear, such as AM-to-PM conversion.

It is important to measure how reflective a component or circuit is, to ensure that it transmits or absorbs energy efficiently. Measuring the complex impedance of an antenna is a good example.

Using the Analyzer's Phase Format

The analyzer's phase format displays a phase-versus-frequency or phase-versus-power measurement. The analyzer does not display more than ± 180 degrees phase difference between the reference and test signals. As the phase value varies between $+180$ degrees and -180 degrees, the analyzer display creates the sawtooth pattern as shown in the following graphic.

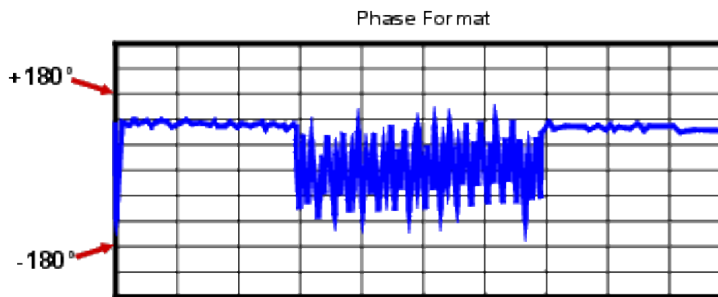

The sawtooth pattern does not always reach $+180$ degrees and -180 degrees. This is because the measurement is made at discrete frequencies, and the data point at $+180$ degrees and -180 degrees may not be measured for the selected sweep.

Types of Phase Measurements

Complex impedance data is information such as resistance, reactance, phase, and magnitude that can be determined from an S11 or S22 measurement. Complex impedance data can be viewed using either the Smith Chart format or the Polar format.

AM-to-PM conversion is a measure of the amount of undesired phase deviation (PM) that is caused by amplitude variations (AM) of the system. AM-to-PM conversion is usually defined as the change in output phase for a 1-dB increment in the input power to an amplifier (i.e. at the 1 dB gain compression point). This is expressed in degrees-

per-dB ($^{\circ}/\text{dB}$).

Deviation from linear phase is a measure of phase distortion caused by a device. Ideally, the phase shift through a device is a linear function of frequency. The amount of variation from this theoretical phase shift is known as its deviation from linear phase (also called phase linearity).

Group delay is another way to look at phase distortion caused by a device. Group delay is a measure of transit time through a device at a particular frequency. The analyzer computes group delay from the derivative of the measured phase response.

Deviation from Linear Phase Versus Group Delay

Although deviation from linear phase and group delay are similar measurements, they each have their purpose.

The following are the advantages of deviation from linear phase measurements:

- Less noisy than group delay.
- Able to characterize devices that pass phase modulated signals, and show units of phase rather than units of seconds.

The following are the advantages of group delay measurements:

- More easily interpreted indication of phase distortion than deviation from linear phase.
- Able to most accurately characterize a device under test. This is because in determining group delay, the analyzer calculates the slope of the phase ripple, which is dependent on the number of ripples which occur per unit of frequency. Comparing two phase responses with equal peak-to-peak phase ripple, the response with the larger phase slope results in:
 - More group delay variation.
 - More signal distortion.

Balanced Measurements

What are Balanced Devices?

Differential and Common Modes Model

Measuring Mixed Mode (Balanced) S-Parameters

Measuring Imbalance Parameters

Measuring CMRR


Port Mapping

How the PNA makes Balanced Measurements


Other Measurement Setup Topics

What are Balanced Devices?

Standard **Single-ended devices** generally have one input port and one output port. Signals on the input and output ports are referenced to ground.

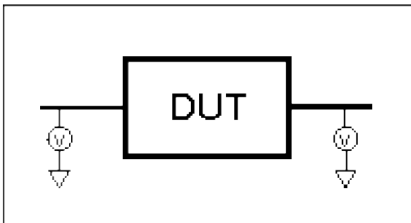

Balanced devices have two pins on either the input, the output, or both. The signal of interest is the difference and average of the two input or output lines, not referenced to ground.

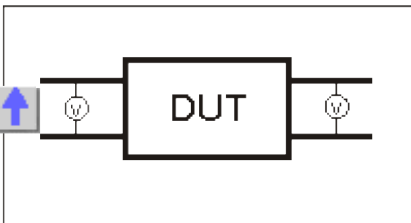


Differential and Common Modes Model

On balanced devices, the signal of interest is the **difference** and **average** of the two input or output lines. In balanced device terminology, these signals are known as the Differential and Common modes.

The following model shows how two signals (A and B) combine to create Differential and Common mode signals:

- **Signal A** is fixed at 1V peak
- **Signal B** is **selectable**
- **Differential** is calculated as **A minus B**
- **Common** is calculated as the **AVERAGE** of **A and B**

Note: Click **Signal B** selections to see various Differential and Common signals.

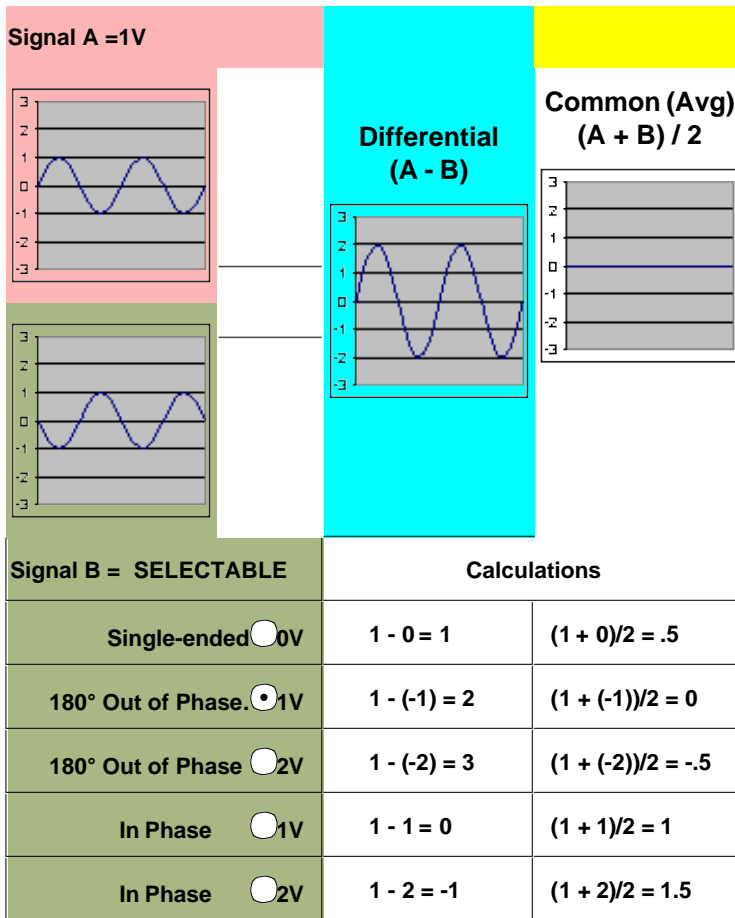

Notes:

- Even when Signal B is 0V, like a Single -ended signal, there is still a unique Differential and Common mode representation of the two individual signals.
- The above model does not show a DUT. The difference and average of two signals can be calculated for both the balanced INPUT and balanced OUTPUT of a device.

Measuring Mixed Mode (Balanced) S-Parameters

Mixed mode S-parameters combine traditional S-parameter notation with balanced measurement terminology.

Some balanced devices are designed to amplify the differential component and reject the common component. This allows noise that is common to both inputs to be virtually eliminated from the output. For example, a balanced device may amplify the differential signal by a factor of 5, and attenuate the common signal by a factor of 5. Using traditional S-parameter notation, an S21 is a ratio measurement of the device **Output** / device **Input**. Mixing this with balanced terminology, we could view the amplifier's Differential Output signal / Differential Input signal. To see this parameter on the PNA, we would select an Sdd21 measurement using the following balanced notation:

Sabxy -

Where

a = output mode

b = input mode

(choose from the following for both a and b:)

- **d** - differential
- **c** - common
- **s** - single ended

x = output "logical" port number

y = input "logical" port number

(see the following regarding "logical" port mapping)

Measuring Imbalance Parameters

Imbalance is a measure of how well two physical ports that make up a balanced port are matched. With a perfectly balanced port, the same amount of energy flows to both ports and the magnitude of the ratio of these ports would be 1.


The notation is similar to traditional S-parameters. In the following diagrams, the letters a, b, c, and d used because any PNA port can be assigned to any logical port in the port mapping process.

S_{xy} -


Where

a = output port


b = input port

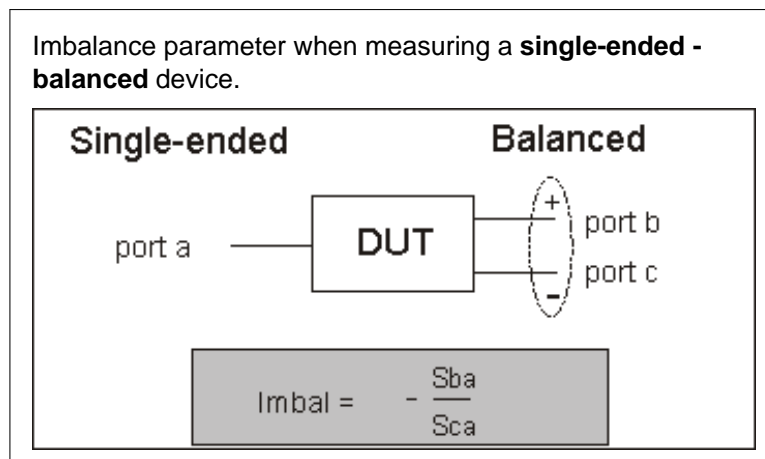

Imbalance1 and Imbalance2 parameters when measuring a **balanced - balanced** device.

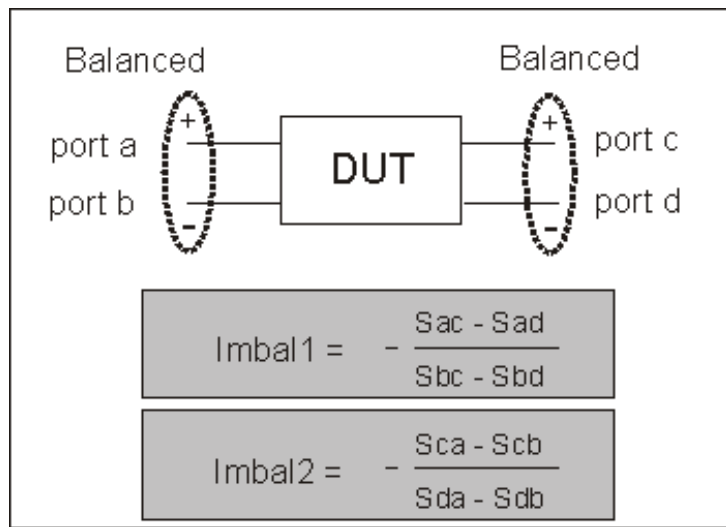

Imbalance1 and Imbalance2 parameters when measuring a **single-ended - single-ended - balanced** device.

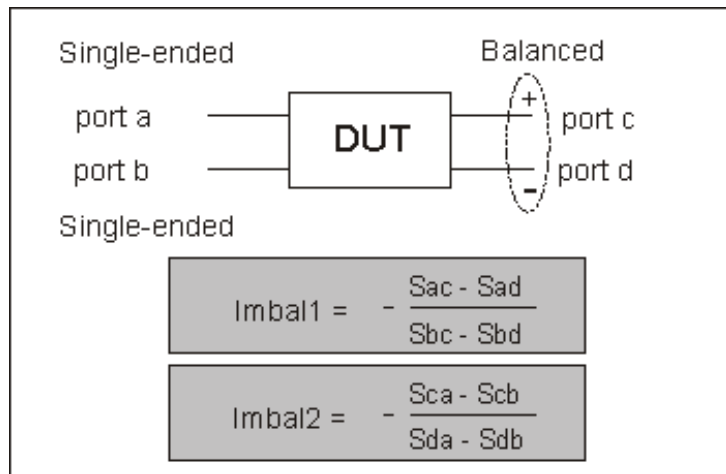

Measuring CMRR (Common Mode Rejection Ratio)


CMRR is a ratio of the transmission characteristic in differential mode over the transmission characteristic in the common mode of the balanced port as the measurement parameter. A high value indicates more rejection of common mode, which is desirable in a device that transmits information in the differential portion of the signal. The table below shows the CMRR parameter you can select when measuring each balanced device.

Single-ended - balanced device	$\frac{S_{ds21}}{S_{cs21}}$ and $\frac{S_{sd12}}{S_{sc12}}$
Balanced - balanced device	$\frac{S_{dd21}}{S_{cc21}}$
Single-ended - single-ended - balanced device	$\frac{S_{ds31}}{S_{cs31}}$ and $\frac{S_{ds32}}{S_{cs32}}$

Device Topology and Port Mapping


As we have seen on balanced inputs and outputs, the signal of interest is the difference or average of two BALANCED input or BALANCED output lines. It is also possible to have single-ended ports AND balanced ports on the same device. The two balanced input or output lines are referred to as a single "logical" port.

When configuring a balanced measurement on the PNA, select a device 'topology'. Then map each PNA test port to the DUT ports. The PNA assigns "logical ports". See how to set device topology in the PNA.

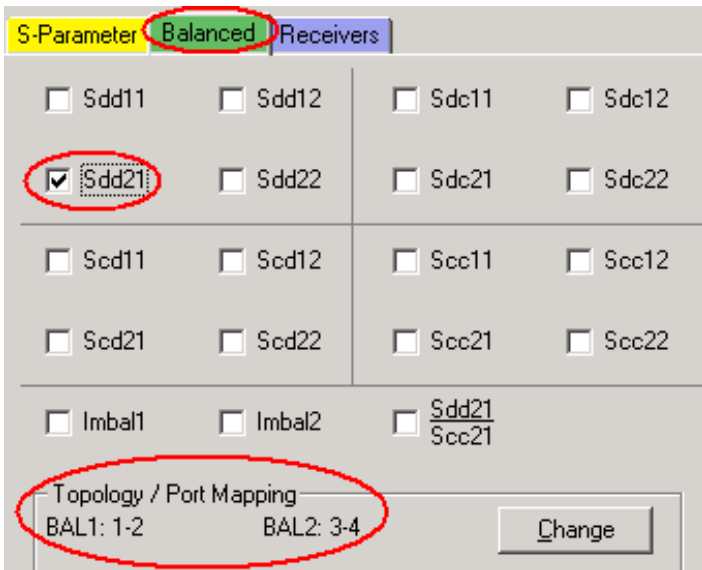


The following device topologies can be measured by a 4-port PNA.


- **Balanced / Balanced**
(2 logical ports - <4 actual ports>)

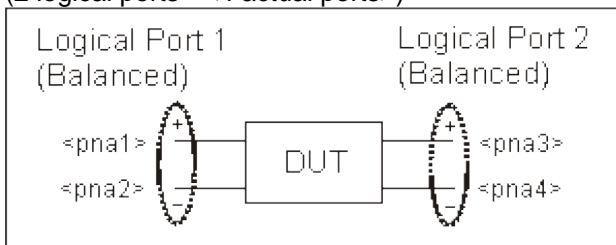

- **Single-ended / Balanced**
(2 logical ports - <3 actual ports>)

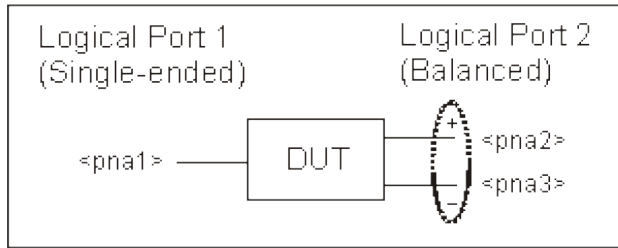

- **Single-ended - Single-ended / Balanced**
(3 logical ports - <4 actual ports>)

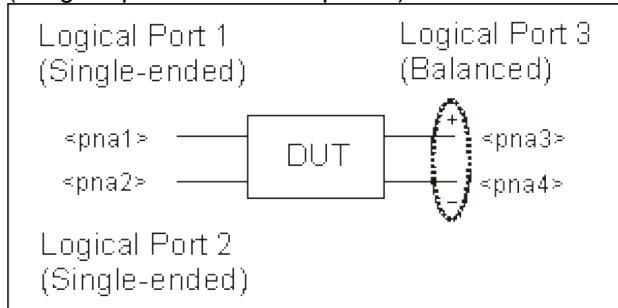

These topologies can be used in the reverse (<==>) direction to measure:

- **Balanced / Single-ended** topology
- **Balanced / Single-ended - Single-ended** topology

For example, to measure a **Balanced / Single-ended** topology, measure the S12 (reverse direction) of a **Single-ended / Balanced** topology.

How the PNA makes Balanced Measurements

The PNA does not provide true balanced measurements by stimulating both balanced inputs together and measuring both outputs relative to one another. Instead, the PNA makes only Single-ended measurements. On a Balanced/ Balanced device, it stimulates each input and measures each output individually. From the output data, the PNA calculates the Differential and Common outputs from the DUT using the same math formulas as the above model. However, all measurements and calculations on the PNA are performed in frequency domain using complex (magnitude and phase) data. The Balanced S-parameter display data is then calculated from the Differential and Common inputs and outputs.

Amplifier Parameters Reference

[Gain](#)

[Gain Flatness](#)

[Reverse Isolation](#)

[Gain Drift Versus Time](#)

[Deviation from Linear Phase](#)

[Group Delay](#)

[Return Loss \(SWR, r\)](#)

[Complex Impedance](#)

[Gain Compression](#)

[AM-to-PM Conversion](#)

Gain

$$\tau = \frac{V_{\text{trans}}}{V_{\text{inc}}}$$

$$\text{Gain (dB)} = -20 \log_{10} |\tau|$$

$$\text{Gain (dB)} = P_{\text{out}} \text{ (dBm)} - P_{\text{in}} \text{ (dBm)}$$

The ratio of the amplifier's output power (delivered to a Z_0 load) to the input power (delivered from a Z_0 source). Z_0 is the characteristic impedance, in this case, 50Ω .

For small signal levels, the output power of the amplifier is proportional to the input power. Small signal gain is the gain in this linear region.

As the input power level increases and the amplifier approaches saturation, the output power reaches a limit and the gain drops. Large signal gain is the gain in this nonlinear region. See [Gain Compression](#).



Gain Flatness

The variation of the gain over the frequency range of the amplifier. See [Small Signal Gain and Flatness](#).

Reverse Isolation

The measure of transmission from output to input. Similar to the gain measurement except the signal stimulus is applied to the output of the amplifier. See [Reverse Isolation](#).

Gain Drift versus Time (temperature, bias)

The maximum variation of gain as a function of time, with all other parameters held constant. Gain drift is also observed with respect to other parameter changes such as temperature, humidity or bias voltage.

Deviation from Linear Phase

The amount of variation from a linear phase shift. Ideally, the phase shift through an amplifier is a linear function of frequency. See [Deviation from Linear Phase](#).

Group Delay

$$\begin{aligned}\tau_g (\text{sec}) &= - \frac{\Delta \theta}{\Delta \omega} \\ &= - \frac{1}{360} * \frac{\Delta \theta}{\Delta f}\end{aligned}$$

The measure of the transit time through the amplifier as a function of frequency. A perfectly linear phase shift would have a constant rate of change with respect to frequency, yielding a constant group delay. See [Group Delay](#).

Return Loss (SWR, r)

$$\begin{aligned}\Gamma &= \frac{V_{\text{refl}}}{V_{\text{inc}}} = \rho \angle \theta \\ \text{Reflection coefficient} &= \rho \\ \text{Return loss (dB)} &= -20 \log_{10} \rho \\ \text{SWR} &= \frac{1+\rho}{1-\rho}\end{aligned}$$

The measure of the reflection mismatch at the input or output of the amplifier relative to the system Z_0 [characteristic impedance](#).

Complex Impedance

$$\begin{aligned}Z &= \frac{1+\Gamma}{1-\Gamma} * Z_0 \\ &= -R + jX\end{aligned}$$

Complex [impedance](#) (1+G). The amount of reflected energy from an amplifier is directly related to its impedance. Complex impedance consists of both a resistive and a reactive component. It is derived from the characteristic impedance of the system and the reflection coefficient. See [Complex Impedance](#).

Gain Compression

An amplifier has a region of linear gain where the gain is independent of input power level (small signal gain). As the power is increased to a level that causes the amplifier to saturate, the gain decreases.

Gain compression is determined by measuring the amplifier's 1 dB gain compression point (P_{1dB}) which is the output power at which the gain drops 1 dB relative to the small signal gain. This is a common measure of an amplifier's power output capability. See [Gain Compression](#).

AM-to-PM Conversion Coefficient

$$\text{AM/PM} = \frac{\Delta \theta}{\Delta P}$$

The amount of [phase](#) change generated in the output signal of an amplifier as a result of an amplitude change of the input signal.

The AM-to-PM conversion coefficient is expressed in units of degrees/dB at a given power level (usually P_{1dB}, which is the 1 dB gain compression point). See [AM-PM Conversion](#).

AM-PM Conversion

The AM-PM conversion of an amplifier is a measure of the amount of undesired phase deviation (PM) that is caused by amplitude variations (AM) inherent in the system.

What Is AM-PM Conversion?

Why Measure AM-PM Conversion

Accuracy Considerations

How to Measure AM-PM Conversion

Other Tutorial topics

What Is AM-PM Conversion?

AM-to-PM conversion measures the amount of undesired phase deviation (PM) that is caused by amplitude variations (AM) of the system. For example, unwanted phase deviation (PM) in a communications system can be caused by:

Unintentional amplitude variations (AM)


- Power supply ripple
- Thermal drift
- Multipath fading

Intentional modulation of signal amplitude

- QAM
- Burst modulation



AM-to-PM conversion is usually defined as the change in output phase for a 1-dB increment in the power-sweep applied to the amplifier's input (i.e. at the 1 dB gain compression point). It is expressed in degrees-per-dB ($^{\circ}/\text{dB}$). An ideal amplifier would have no interaction between its phase response and the power level of the input signal.

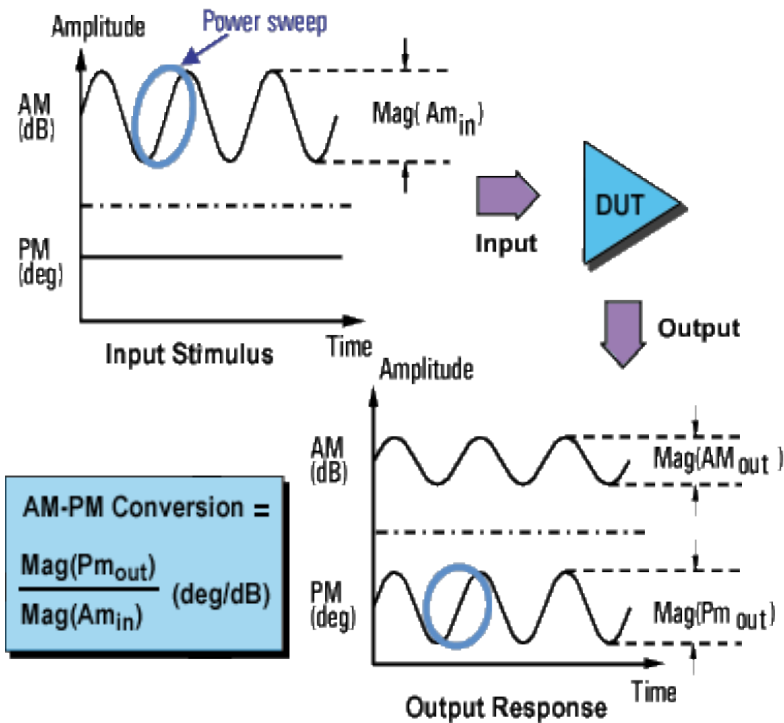


Why Measure AM-PM Conversion

AM-to-PM conversion is a critical parameter in systems where phase (angular) modulation is used, such as:

- FM
- QPSK
- 16QAM

It is a critical parameter because undesired phase deviation (PM) causes analog signal degradation, or increased bit-error rates (BER) in digital communication systems. While it is easy to measure the BER of a digital communication system, this measurement alone does not help you understand the underlying causes of bit errors. AM-to-PM conversion is one of the fundamental contributors to BER, and therefore it is important to quantify this parameter in communication systems.

Refer to the I/Q diagram below for the following discussion on how AM-to-PM conversion can cause bit errors.

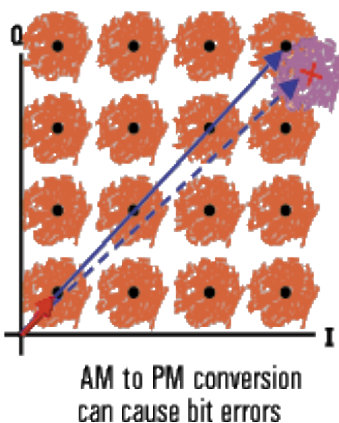

- The desirable state change is from the small solid vector to the large solid vector.

- With AM-to-PM conversion, the large vector may actually end up as shown with the dotted line. This is due to phase shift that results from a change in the input power level.
- For a 64QAM signal as shown (only one quadrant is drawn), we see that the noise circles that surround each state would actually overlap, which means that statistically, some bit errors would occur.


Accuracy Considerations

With this method of measuring AM-to-PM conversion, the modulation frequency is approximately the inverse of the sweep time. Even with the fastest power sweep available on most network analyzers, the modulation frequency ends up being fairly low (typically less than 10 Hz). This could cause a slight temperature change as the sweep progresses, especially if the amplifier has low thermal mass, typical of an unpackaged device. Results using this method could differ slightly if the nonlinear behavior of an amplifier is extremely sensitive to thermal changes. (The PNA series analyzers can make power sweeps <1 ms.)

- The amplifier may respond very differently at various temperatures. The tests should be done when the amplifier is at the desired operating temperature.
- The output power of the amplifier should be sufficiently attenuated if necessary. Too much output power could:
 - damage the analyzer receiver
 - exceed the input compression level of the analyzer receiver, resulting in inaccurate measurements
- Attenuation of the amplifier's output power can be accomplished using:
 - Attenuators
 - Couplers
- The frequency-response effects of the attenuators and couplers must be accounted for during calibration since they are part of the test system. Proper error-correction techniques can reduce these effects.
- The frequency response is the dominant error in an AM-to-PM conversion measurement setup. Performing a thru-response measurement calibration significantly reduces this error. For greater accuracy, perform a 2-port measurement calibration.

How to Measure AM-PM Conversion

1. Preset the analyzer.
2. Select an S21 measurement in the power-sweep mode.
3. Enter the start and stop power levels for the analyzer's power sweep. The start power level should be in the linear region of the amplifier's response (typically 10-dB below the 1-dB compression point). The stop power should be in the compression region of the amplifier's response.
4. Select an external attenuator (if needed) so the amplifier's output power will be sufficiently attenuated to avoid causing receiver compression or damage to the analyzer's port 2.
5. Connect the amplifier as shown in the following graphic, and provide the dc bias.

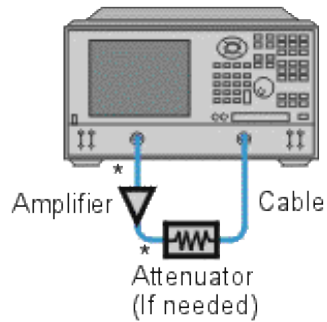

* Direct Connection

6. Select the analyzer settings for your amplifier under test in order to perform a swept-power gain compression measurement at a chosen frequency. See [Gain Compression](#).
7. Remove the amplifier and perform a measurement calibration. Be sure to include the attenuator and cables in the calibration setup if they will be used when measuring the amplifier.
8. Save the instrument state to memory.
9. Reconnect the amplifier.
10. Use a reference marker to target the amplifier's input power at the 1-dB gain compression point. Select a second marker and adjust its stimulus value until its response is 1-dB below the reference marker.
11. Change the S_{21} measurement from a log magnitude format to a [phase](#) format (no new calibration is required).
12. Find the [phase](#) change between the markers. The value is the AM-to-PM conversion coefficient at the 1-dB gain compression point.
13. Print the data or save it to a disk.

Antenna Measurements

This topic describes how to setup the PNA to make S21 measurements on an array of antennas. Measurements can be made on up to 100 antenna arrays (Ports) and up to 15 discrete frequencies

Measurement Sequence

1. The PNA is set to a start frequency.
2. As the antenna moves, the PNA responds to each external trigger signal by measuring an antenna port.
3. When all ports are measured, the PNA increments to the next frequency
4. Again the PNA measures all ports, and so forth until all ports are measured at all frequencies in the forward direction.
5. As the antenna begins moving in the opposite direction, the same sequence occurs, except the PNA decrements in frequency until all ports are measured at all frequencies and the PNA is set back to the original start frequency.

Once setup, only external trigger signals are sent to the PNA. After each trigger, measurement data is stored in internal PNA memory.

How to set up the PNA

See the [Antenna Macro](#) to learn how to do this automatically.

1. On the **System** menu click **Preset**
2. On the **Sweep** menu point to **Trigger** then click **Trigger**
3. In Trigger Source click **External**
4. In Trigger Scope click **Channel**
5. Click **OK**

Forward Sweep

1. On the **Trace** menu click **New Trace**
2. Click **S21** then Channel Number **1**
3. On the **Sweep** menu point to **Trigger** then click **Trigger**
4. In Channel Trigger State check **Point Sweep**
5. Click **OK**
6. On the Sweep menu click **Sweep Type:**then **Segment Sweep**
7. Click **OK**

8. On the **View** menu point to **Tables** then click **Segment Table**
9. Do this 15 times - Sweep menu point to **Segment Table** then **Insert Segment**
10. For each Segment in the Segment table:
 1. Click **State**:and select **ON**
 2. Double click both **START** and **STOP** Frequency: (each new segment ascends in frequency)
 3. Double click **Points**: type Number of Ports (elements)

Reverse sweep

Repeat the following steps for each frequency: (up to 15)

- Increment the channel number (**X**) Starting with Channel 2
 - Decrement the frequency (**F**)
1. On the **Trace** menu click **New Trace...**
 2. Click **S21** then Channel Number **X**
 3. When a window contains four traces, check **Create in New Window**.
 4. Click **OK**
 5. On the **Sweep** menu point to **Trigger** then click **Trigger**
 6. In Channel Trigger State check **Point Sweep**
 7. Click **OK**
 8. On the Sweep menu click **Sweep Type**:then **Segment Sweep**
 9. Click **OK**
 10. On the **View** menu point to **Tables** then click **Segment Table**
 11. In the Segment table
 1. Click **State**:and select **ON**
 2. Double click both **START** and **STOP** Frequency **F**
 3. Double click **Points**: type Number of Ports (elements)

Antenna Test Macro

This VB Script macro automates the setup of a PNA as documented in [Antenna Measurements](#). This topic will show you how to copy this macro into a PNA and then run the macro.

For more information, see [Using Macros](#).

Note: Print these instructions if viewing in the PNA. This topic will be covered by the Macro Setup dialog box.

1. Copy the following code into a [Notepad](#) file.

```
'Start copying here
Set rfna = CreateObject("AgilentPNA835x.Application")
Set chans = rfna.Channels
numfreqs = 15
portz = 3
rfna.Preset
rfna.Reset
rfna.TriggerSignal=3 ' Manual trigger
rfna.TriggerType=1 ' ChannelTrigger
'setup forward sweep
win = 1
trce = 1
rfna.CreateMeasurement 1, "S21", 2, win
Set chan = rfna.ActiveChannel
chan.TriggerMode = 0 'TriggerModePoint
chan.SweepType = 4 'SegmentSweep

For i = 1 To 15
chan.Segments.Add (i)
chan.Segments(i).State = True
chan.Segments(i).NumberOfPoints = portz
Next

chan.Segments(1).StartFrequency = 30000
chan.Segments(1).StopFrequency = 30000
chan.Segments(2).StartFrequency = 1000000
chan.Segments(2).StopFrequency = 1000000
chan.Segments(3).StartFrequency = 500000
chan.Segments(3).StopFrequency = 500000
chan.Segments(4).StartFrequency = 10000000
chan.Segments(4).StopFrequency = 10000000
chan.Segments(5).StartFrequency = 100000000
chan.Segments(5).StopFrequency = 100000000
chan.Segments(6).StartFrequency = 500000000
chan.Segments(6).StopFrequency = 500000000
chan.Segments(7).StartFrequency = 1000000000
chan.Segments(7).StopFrequency = 1000000000
chan.Segments(8).StartFrequency = 2000000000
chan.Segments(8).StopFrequency = 2000000000
chan.Segments(9).StartFrequency = 3000000000
chan.Segments(9).StopFrequency = 3000000000
chan.Segments(10).StartFrequency = 4000000000
chan.Segments(10).StopFrequency = 4000000000
chan.Segments(11).StartFrequency = 5000000000
chan.Segments(11).StopFrequency = 5000000000
```

```

chan.Segments(12).StartFrequency = 6000000000
chan.Segments(12).StopFrequency = 6000000000
chan.Segments(13).StartFrequency = 7000000000
chan.Segments(13).StopFrequency = 7000000000
chan.Segments(14).StartFrequency = 8000000000
chan.Segments(14).StopFrequency = 8000000000
chan.Segments(15).StartFrequency = 9000000000
chan.Segments(15).StopFrequency = 9000000000

'setup reverse sweep
'setup the channel
'start with ch 2
For ch = 2 To numfreqs + 1

'put four traces per window
trce = trce + 1
If trce = 5 Then
win = win + 1
trce = 1
End If

rfna.CreateMeasurement ch, "S21", 2, win

Set chan = rfna.ActiveChannel
chan.TriggerMode = 0 'TriggerModePoint
chan.SweepType = 4 'SegmentSweep
Set segs = chan.Segments

Select Case ch
Case 2
segs(1).StartFrequency = 9000000000
segs(1).StopFrequency = 9000000000
Case 3
segs(1).StartFrequency = 8000000000
segs(1).StopFrequency = 8000000000
Case 4
segs(1).StartFrequency = 7000000000
segs(1).StopFrequency = 7000000000
Case 5
segs(1).StartFrequency = 6000000000
segs(1).StopFrequency = 6000000000
Case 6
segs(1).StartFrequency = 5000000000
segs(1).StopFrequency = 5000000000
Case 7
segs(1).StartFrequency = 4000000000
segs(1).StopFrequency = 4000000000
Case 8
segs(1).StartFrequency = 3000000000
segs(1).StopFrequency = 3000000000
Case 9
segs(1).StartFrequency = 2000000000
segs(1).StopFrequency = 2000000000
Case 10
segs(1).StartFrequency = 1000000000
segs(1).StopFrequency = 1000000000
Case 11

```



```

segs(1).StartFrequency = 50000000
segs(1).StopFrequency = 50000000
Case 12
segs(1).StartFrequency = 100000000
segs(1).StopFrequency = 100000000
Case 13
segs(1).StartFrequency = 10000000
segs(1).StopFrequency = 10000000
Case 14
segs(1).StartFrequency = 500000
segs(1).StopFrequency = 500000
Case 15
segs(1).StartFrequency = 100000
segs(1).StopFrequency = 100000
Case 16
segs(1).StartFrequency = 30000
segs(1).StopFrequency = 30000
End Select

segs(1).NumberOfPoints = portz
Next

'End copying here


```

2. Save the file on the analyzer hard drive in the **C:\Documents** folder. Name the file **AntennaTest.vbs** . If viewing this on an external PC, you can transfer the file to the PNA with a floppy disk or by mapping a drive.
3. Close Notepad

Load the macro into the analyzer

1. In the analyzer application, click **System**, point to **Macro**, then click **Macro Setup**
2. Click on a blank line below the last entry. (There may be NO entry.)
3. Click **Edit**
4. In the **Macro Title** box, type **Antenna Test**
5. Click **Browse**.
6. Change **Files of Type** to **VBScript** Go to the **C:\Documents** folder.
7. Click **AntennaTest.vbs**
8. Click **OK**
9. Click **OK** on the Macro Setup dialog box.

To run the macro:

1. Press  on the Front Panel **UTILITY** keys.
2. Click the Active Entry key labeled **Antenna Test**

Complex Impedance

When making an S_{11} or S_{22} measurement of your device under test, you can view complex-impedance data such as series resistance and reactance as well as phase and magnitude information. Complex impedance data can be viewed using either the Smith Chart format or the Polar format.

[What Is Complex Impedance?](#)

[Accuracy Considerations](#)

[How to Measure Complex Impedance](#)

What Is Complex Impedance?

Complex-impedance data is information that can be determined from an S_{11} or S_{22} measurement of your device under test, such as:

- Resistance
- Reactance
- Phase
- Magnitude

The amount of power reflected from a device is directly related to the impedances of both the device and the measuring system. For example, the value of the complex reflection coefficient (Γ) is equal to 0 only when the device impedance and the system impedance are exactly the same (i.e. maximum power is transferred from the source to the load). Every value for Γ corresponds uniquely to a complex device impedance (as a function of frequency), according to the equation:

$$Z_L = [(1 + \Gamma) / (1 - \Gamma)] \times Z_0$$


where Z_L is your test device impedance and Z_0 is the measuring system's characteristic impedance.

Complex Impedance is best viewed using either [Polar](#) or [Smith Chart](#) format.

Accuracy Considerations

- The Smith chart is most easily understood when used with a full scale value of 1.0.
- For greater accuracy when using markers in the Smith chart or polar formats, activate the discrete marker mode.
- The uncertainty of reflection measurements is affected by:
 - [Directivity](#)
 - Reflection tracking
 - Source match
 - [Load match](#) (with 2-port devices)

With a 2-port [calibration](#), the effects of these factors are reduced. A 1-port calibration provides the same accuracy if the output of the device is well terminated. Refer to the graphic below for the following discussion.

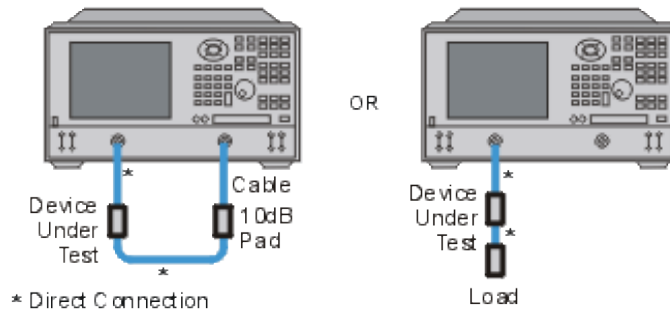

- If you connect the device between both analyzer ports, it is recommended that you use a 10 dB pad on the output of the device to improve measurement accuracy. This is not necessary if you use a 2-port calibration since it corrects for load match.
- If you connect a two-port device to only one analyzer port, it is recommended that you use a high-quality load (such as a calibration standard) on the output of the device.

How to Measure Complex Impedance

1. Connect the device as shown in the previous graphic.
2. Preset the analyzer.
3. Set up, calibrate, and perform an S11 or S22 measurement.
4. View impedance data:
 - a. Select the Smith Chart format.
 - b. Scale the displayed measurement for optimum viewing.
 - c. Position the marker to read the resistive and reactive components of the complex impedance at any point along the trace.
 - d. Print the data or save it to a disk.
5. View the magnitude and phase of the reflection coefficient:
 - a. Select the Smith chart format or the Polar format.
 - b. Select either Lin Marker or Log Marker formats.
 - c. Scale the displayed measurement for optimum viewing.
 - d. Position the marker to read the frequency, magnitude, and phase of the reflection coefficient (Γ) at any point along the trace.
 - e. Print the data or save it to a disk.

Deviation from Linear Phase

Deviation from linear phase is a measure of phase distortion. The electrical delay feature of the analyzer is used to remove the linear portion of the phase shift from the measurement. This results in a high-resolution display of the non-linear portion of the phase shift (deviation from linear phase).

[What Is Linear Phase Shift?](#)

[What Is Deviation from Linear Phase?](#)

[Why Measure Deviation from Linear Phase?](#)

[Using Electrical Delay](#)

[Accuracy Considerations](#)


[See other Tutorials](#)

What Is Linear Phase Shift?

Phase shift occurs because the wavelengths that occupy the electrical length of the device get shorter as the frequency of the incident signal increases. *Linear* phase-shift occurs when the phase response of a device is linearly proportional to frequency. Displayed on the analyzer, the phase-versus-frequency measurement trace of this ideal linear phase shift is a straight line. The slope is proportional to the electrical length of the device. Linear phase shift is necessary (along with a flat magnitude response) for distortionless transmission of signals.

What Is Deviation from Linear Phase?

In actual practice, many electrical or electronic devices will delay some frequencies more than others, creating non-linear phase-shift (distortion in signals consisting of multiple-frequency components). Measuring deviation from linear phase is a way to quantify this non-linear phase shift.

Since it is only the deviation from linear phase which causes phase distortion, it is desirable to remove the linear portion of the phase response from the measurement. This can be accomplished by using the electrical delay feature of the analyzer to mathematically cancel the electrical length of the device under test. What remains is the  deviation from linear phase, or phase distortion.

Why Measure Deviation from Linear Phase?

The deviation from linear phase measurement accomplishes the following:

- Presents data in units of phase rather than units of seconds (group delay). For devices that pass modulated signals, units of phase may be most practical.
- Provides a less noisy measurement than a group delay measurement.


Using Electrical Delay

The electrical delay feature is the electronic version of the mechanical "line stretcher" of earlier analyzers. This feature does the following:

- Simulates a variable-length lossless transmission line, which is effectively added to or removed from the

reference signal path.

- Compensates for the electrical length of the device under test.
- Flattens the measurement trace on the analyzer's display. This allows the trace to be viewed at high resolution in order to see the details of the phase nonlinearity.
- Provides a convenient method to view the deviation from linear phase of the device under test. See the following graphic.

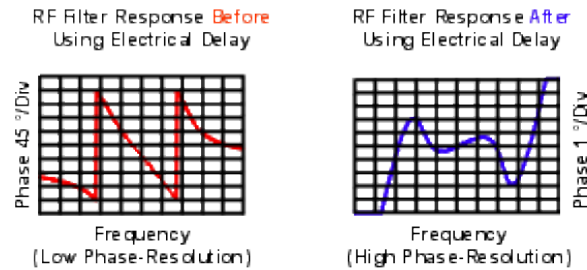


Accuracy Considerations

The frequency response of the test setup is the dominant error in a deviation from linear phase measurement. Performing a thru-response measurement calibration significantly reduces this error. For greater accuracy, perform a 2-port measurement calibration.

How to Measure Deviation from Linear Phase:

1. Preset the analyzer.
2. If your device under test is an amplifier, it may be necessary to adjust the analyzer's source power:
 - Set the analyzer's source power to be in the linear region of the amplifier's output response (typically 10-dB below the 1-dB compression point).
 - Select an external attenuator (if needed) so the amplifier's output power will be sufficiently attenuated to avoid causing receiver compression or damage to the analyzer's port 2.
3. Connect the device under test as shown in the following graphic.

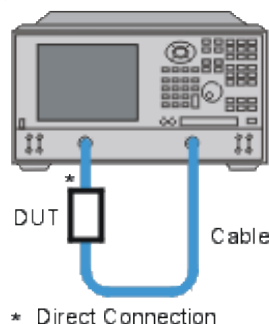

3. Select an S21 measurement.
4. Select the settings for your device under test, including the following:

- Format: phase
 - Scale: autoscale
5. Remove the device and perform a calibration.
 6. Reconnect the device.
 7. Scale the displayed measurement for optimum viewing.
 8. Activate the electrical delay function to automatically flatten the phase trace. If desired, manually fine-tune electrical delay to adjust the flatness of the phase trace.
 9. Use the markers to measure the maximum peak-to-peak deviation from linear phase.
 10. Print the data or save it to a disk.

Group Delay

Group delay is a measure of phase distortion. Group delay is the actual transit time of a signal through a device under test as a function of frequency. When specifying group delay, it is important to specify the aperture used for the measurement.

What is Group Delay?

Group Delay versus Deviation from Linear Phase

What Is Aperture?

Accuracy Considerations

How to Measure Group Delay


See other Amplifier Parameter topics

What Is Group Delay?

Group delay is:

- A measure of device phase distortion.
- The transit time of a signal through a device, versus frequency.
- The derivative of the device's phase characteristic with respect to frequency.

Refer to the graphic below for the following discussion:

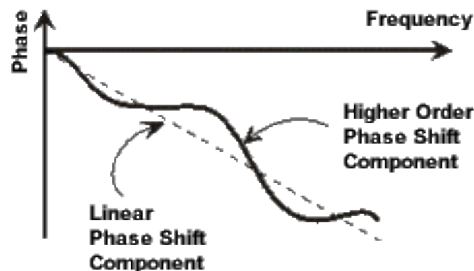

$$\begin{aligned} \text{Group Delay} = t_g &= \frac{-d\phi}{d\omega} && \phi \text{ in Radians} \\ &&& \omega \text{ in Radians/Sec} \\ &= \frac{-1}{360^\circ} \cdot \frac{d\Theta}{df} && \Theta \text{ in Degrees} \\ &&& f \text{ in Hz } (\omega = 2\pi f) \end{aligned}$$

The phase characteristic of a device typically consists of both linear and higher order (deviations from linear) phase-shift components.

Linear phase-shift component:

Represents average signal transit time.


Attributed to electrical length of test device.

Higher-order phase-shift component:

Represents variations in transit time for different frequencies.

Source of signal distortion.

Refer to the graphic below for the following discussion:

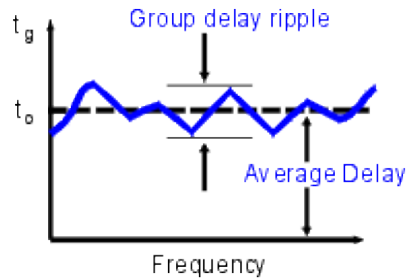

In a group delay measurement:

- The linear phase shift component is converted to a constant value (representing the average delay).
- The higher order phase shift component is transformed into deviations from constant group delay (or group delay ripple).
- The deviations in group delay cause signal distortion, just as deviations from linear phase cause distortion.
- The measurement trace depicts the amount of time it takes for each frequency to travel through the device under test.

Refer to the following equation for this discussion on how the analyzer computes group delay:

$$\text{Group Delay} = t_g = \frac{-d\phi}{d\omega}$$

$$= \frac{-1}{360^\circ} \cdot \frac{d\Theta}{df}$$


ϕ in Radians
 ω in Radians/Sec
 Θ in Degrees
 f in Hz ($\omega = 2\pi f$)

- Phase data is used to find the phase change ($-d\phi$).
- A specified frequency aperture is used to find the frequency change ($d\omega$).
- Using the two values above, an approximation is calculated for the rate of change of phase with frequency.
- This approximation represents group delay in seconds (assuming linear phase change over the specified frequency aperture).

Group Delay versus Deviation from Linear Phase

Group delay is often a more accurate indication of phase distortion than Deviation from Linear Phase.

Deviation from linear phase results are shown in the upper region of the following graphic: Device 1 and device 2 have same value, despite different appearances.

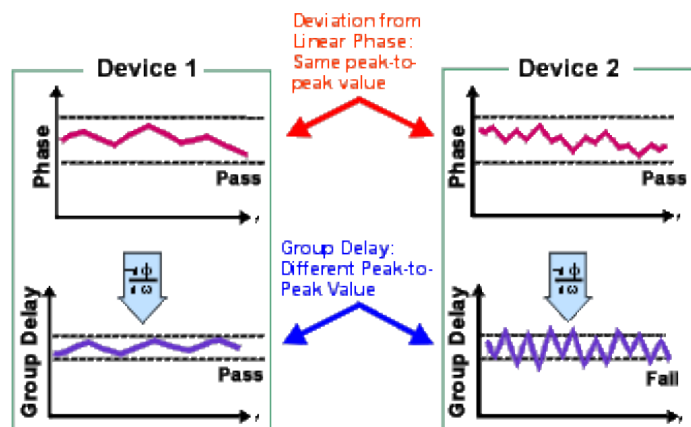


Group Delay results are shown in the lower region:

Device 1 and device 2 have different values of group delay. This is because in determining group delay, the analyzer calculates slope of phase ripple, which is dependent on number of ripples which occur per unit of frequency.

What Is Aperture?

During a group delay measurement, the analyzer measures the phase at two closely spaced frequencies and then computes the phase slope. The frequency interval (frequency delta) between the two phase measurement points is called the aperture. Changing the aperture can result in different values of group delay. The computed slope (delta phase) varies as the aperture is increased. This is why when you are comparing group delay data, you must know the aperture that was used to make the measurements.

Refer to the graphic below for the following discussion:

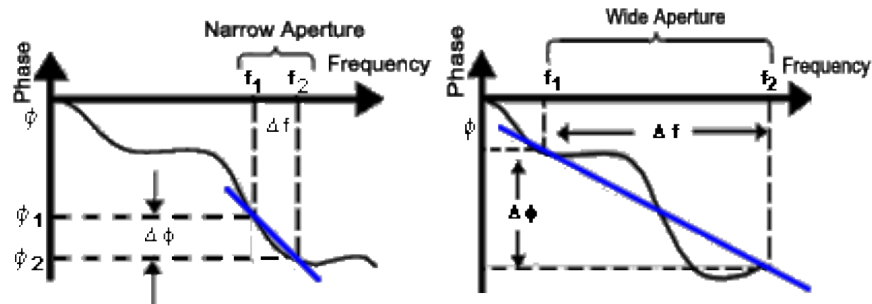

Narrow aperture:

Provides more fine detail in phase linearity.

Makes measurement susceptible to noise (smaller signal-to-noise ratio) and analyzer phase detector resolution.

Wide aperture:

Provides less fine detail in phase linearity because some phase response averaged-out or not measured.

Makes measurement less susceptible to noise (larger signal-to-noise ratio).

The analyzer's default setting for group delay aperture is the frequency span divided by the number of points across the display. There are two ways to set the aperture to a different value.

1. Adjust the number of measurement points or the frequency span.
 - Increasing the number of points or reducing the frequency span narrows the aperture.
 - Decreasing the number of points and/or increasing the frequency span widens the aperture.

Note: if the aperture is too wide (more than 180° of phase shift between adjacent frequency points), errors in group delay data will occur.

2. Use the analyzer's smoothing function.
 - Performs a single-sweep, moving average of adjacent data-points over a specified percentage of the frequency span.
 - Results in an action similar to changing the frequency interval between points.
 - Allows a wider aperture because greater than 180° of phase shift can occur over the smoothing aperture.

Group delay measurements can be made on the following sweep types:

- Linear frequency

- List frequency sweep segment


The group delay aperture varies depending on the frequency spacing and point density, therefore the aperture is not constant in segment sweep. In segment sweep, extra frequency points can be defined to ensure the desired aperture.

Accuracy Considerations

It is important to keep the phase difference between two adjacent measurement points less than 180° (see the following graphic). Otherwise, incorrect phase and delay information may result. Undersampling may occur when measuring devices with long electrical length. You can verify that the phase difference measured between two adjacent points is less than 180° by adjusting the following settings until the measurement trace no longer changes:

- Increase the number of points
- Narrow the frequency span

Electrical delay may also be used to compensate for this effect.

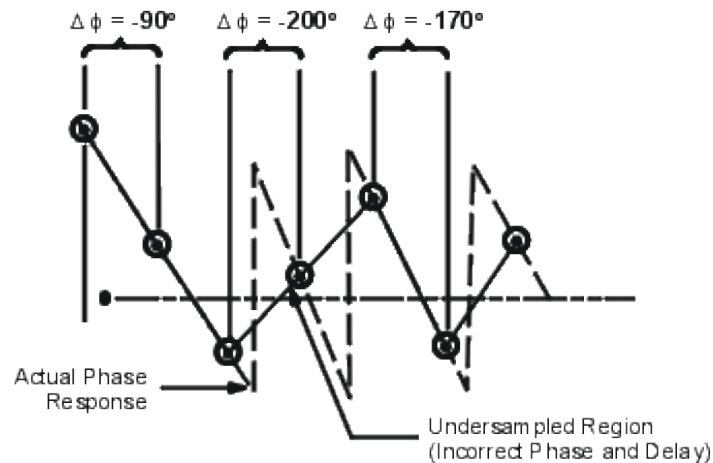


The frequency response is the dominant error in a group delay test setup. Performing a thru-response measurement calibration significantly reduces this error. For greater accuracy, perform a 2-port measurement calibration.

Particularly for an amplifier, the response may vary differently at various temperatures. The tests should be done when the amplifier is at the desired operating temperature.

How to Measure Group Delay

1. Preset the analyzer.
2. If your device under test is an amplifier, it may be necessary to adjust the analyzer's source power:
 - Set the analyzer's source power to be in the linear region of the amplifier's output response (typically 10-dB below the 1-dB compression point).
 - Select an external attenuator (if needed) so the amplifier's output power will be sufficiently attenuated to avoid causing receiver compression or damage to the analyzer's port 2.
3. Connect the device under test as shown in the following graphic.

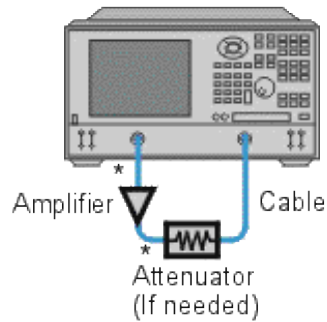

* Direct Connection

4. Select an S₂₁ measurement.
5. Select the settings for your device under test, including the following:
 - number of measurement points: maximum
 - format: delay
 - scale: autoscale
6. Remove the device under test and perform a measurement calibration.
7. Reconnect the device under test.
8. Scale the displayed measurement for optimum viewing.
9. Use the analyzer's smoothing feature to increase the aperture, reducing noise on the trace while maintaining meaningful detail. To increase the aperture:
 - Switch on the analyzer's smoothing feature.
 - Vary the smoothing aperture (up to 25% of the span swept).
10. Use the markers to measure group delay (expressed in seconds) at a particular frequency of interest.
11. Print the data or save it to a disk.

Small Signal Gain and Flatness

Small signal gain is the gain in the amplifier's linear region of operation. This is typically measured at a constant input power over a swept frequency. Gain flatness is the measure of the variation of gain over a specified frequency range.

[What Is Gain?](#)

[What Is Flatness?](#)

[Why Measure Gain and Flatness?](#)

[Accuracy Considerations](#)

[How to Measure Gain and Flatness](#)

[See other Amplifier Parameter topics](#)

What Is Gain?

RF amplifier gain is defined as the difference in power between the amplifier output signal and the input signal. It is assumed that both input and output impedances of the amplifier are the same as the characteristic impedance of the system.

- Gain is called S_{21} using S-parameter terminology
- Gain is expressed in dB—a logarithmic ratio of the output power relative to the input power.
- Gain can be calculated by subtracting the input from the output levels when both are expressed in dBm, which is power relative to 1 milliwatt.
- Amplifier gain is most commonly specified as a minimum value over a specified frequency range. Some amplifiers specify both minimum and maximum gain, to ensure that subsequent stages in a system are not under or over driven.



What Is Flatness?

Flatness specifies how much the amplifier's gain can vary over the specified frequency range. Variations in the flatness of the amplifier's gain can cause distortion of signals passing through the amplifier.

Why Measure Small-Signal Gain and Flatness?

Deviations in gain over the bandwidth of interest will induce distortion in the transmitted signal because frequency components are not amplified equally. Small-signal gain allows you to quantify the amplifier's gain at a particular frequency in a 50-ohm system. Flatness allows you to view the deviations in the amplifier's gain over a specified frequency range in a 50-ohm system.

Accuracy Considerations

- The amplifier may respond very differently at various temperatures. The tests should be done when the amplifier is at the desired operating temperature.

- The output power of the amplifier should be sufficiently attenuated if necessary. Too much output power could:
 - damage the analyzer receiver
 - exceed the input compression level of the analyzer receiver, resulting in inaccurate measurements.

Attenuation of the amplifier's output power can be accomplished using:


- attenuators
- couplers

The frequency-response effects and mismatches of the attenuators and couplers must be accounted for during calibration since they are part of the test system. Proper error-correction techniques can reduce these effects.

- The frequency response is the dominant error in a small-signal gain and flatness measurement setup. Performing a thru-response measurement calibration significantly reduces this error. For greater accuracy, perform a 2-port measurement calibration.
- Reducing IF bandwidth or using averaging improves measurement dynamic range and accuracy, at the expense of measurement speed.

How to Measure Gain and Flatness

1. Preset the analyzer.
2. Select an S21 measurement parameter.
3. Set the analyzer's source power to be in the linear region of the amplifier's output response (typically 10-dB below the 1-dB compression point).
4. Select an external attenuator (if needed) so the amplifier's output power will be sufficiently attenuated to avoid causing receiver compression or damage to the analyzer's port-2.

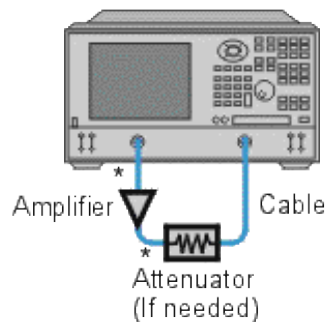

* Direct Connection

5. Connect the amplifier as shown in the following graphic, and provide the dc bias.
6. Select the analyzer settings for your amplifier under test.
7. Remove the amplifier and perform a measurement calibration. Be sure to include the attenuator and cables in the calibration setup if they will be used when measuring the amplifier.

8. Save the instrument-state to memory.
9. Reconnect the amplifier.
10. Scale the displayed measurement for optimum viewing and use a marker to measure the small signal gain at a desired frequency.
11. Measure the gain flatness over a frequency range by using markers to view the peak-to-peak ripple.
12. Print or save the data to a disk.
13. This type of measurement can be automated.

Gain Compression

Gain compression measures the level of input power applied to an amplifier that will cause a distorted output.

What Is Gain Compression?

Why Measure Gain Compression?

Accuracy Considerations


How to Measure Gain Compression

[See other Amplifier Parameter topics](#)

What Is Gain Compression?

Gain compression occurs when the input power of an amplifier is increased to a level that reduces the gain of the amplifier and causes a nonlinear increase in output power.

The analyzer has the ability to do power sweeps as well as frequency sweeps. Power sweeps help characterize the nonlinear performance of an amplifier. Refer to the graphic below (a plot of an amplifier's output power versus input power at a single frequency) for the following discussion.

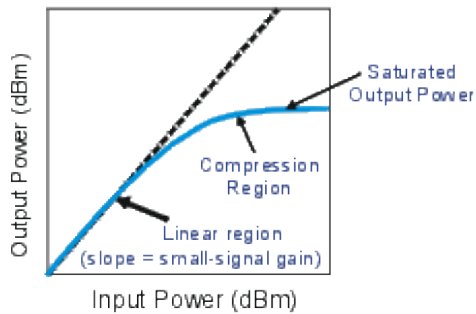

- The amplifier has a linear region of operation where gain is constant and independent of power level. The gain in this region is commonly referred to as "small-signal gain."
- As the input power increases, the amplifier gain appears to decrease, and the amplifier goes into compression.
- The most common measurement of amplifier compression is the 1-dB compression point. This is defined as the input power (or sometimes the output power) which results in a 1-dB decrease in amplifier gain (relative to the amplifier's small-signal gain).

Why Measure Gain Compression?

When driven with a sinusoid, the output of an amplifier is no longer sinusoidal in the compression region. Some of the amplifier output appears in harmonics, rather than occurring only at the fundamental frequency of the input signal.

As input power is increased even more, the amplifier becomes saturated, and output power remains constant. At this point, further increases in amplifier input power result in no change in output power.

In some cases (such as with TWT amplifiers), output power actually decreases with further increases in input power after saturation, which means the amplifier has negative gain.

Since gain is desired in amplifier operation, it is important to know the limit of input signal that will result in gain compression.

Accuracy Considerations

The network analyzer must provide sufficient power to drive the amplifier into saturation. If you need a higher input-power level than the source of the analyzer can provide, use a preamplifier to boost the power level prior to the amplifier under test. (See [High-Power Component Measurements](#).) If using a preamplifier, you can increase measurement accuracy in the following ways:

- Use a coupler on the output of the preamplifier so that a portion of the boosted input signal can be used for the analyzer's reference channel. This configuration removes the preamplifier's [frequency response](#) and drift errors from the measurement (by ratioing).
- Perform a thru-response [calibration](#) including the preamplifier, couplers, and attenuators in the test setup.

The output power of the amplifier should be sufficiently attenuated if necessary. Too much output power could:

- Damage the analyzer receiver
- Exceed the input compression level of the analyzer receiver

[Attenuation](#) of the amplifier's output power can be accomplished using:

- Attenuators
- Couplers

The frequency-response effects of the attenuators and couplers must be considered during calibration since they are part of the test system. Proper error-correction techniques can reduce these effects.

- The frequency response is the dominant error in a gain compression measurement setup. Performing a thru-response measurement calibration significantly reduces this error.
- The amplifier may respond very differently at various temperatures. The tests should be done when the amplifier is at the desired operating temperature.
- Reducing IF [bandwidth](#) or using measurement averages improves accuracy, at the expense of measurement speed.

How to Measure Gain Compression


This procedure shows you how to make the following three measurements used to determine amplifier gain compression:

1. A [Swept-Frequency Gain Compression](#) measurement locates the lowest frequency at which the 1-dB gain compression first occurs.
2. A [Swept-Power Gain Compression](#) measurement shows the input power at which a 1-dB drop in gain occurs as a power ramp is applied to the amplifier at a particular frequency point (found in measurement 1).
3. An [Absolute Power](#) measurement shows the absolute power out (in dBm) at compression.

Swept-Frequency Gain Compression Measurement

A measurement of swept frequency gain compression locates the frequency point where 1-dB compression first occurs.

1. Preset the analyzer.
2. Select an S_{21} measurement parameter.
3. Set the analyzer's source power to be in the linear region of the amplifier's output response (typically 10-dB below the 1-dB compression point).
4. Select an external attenuator (if needed) so the amplifier's output power will be sufficiently attenuated to avoid causing receiver compression or damage to the analyzer's port-2.
5. Connect the amplifier as shown in the following graphic, and provide the dc bias.
6. Select the analyzer settings for your amplifier under test. To reduce the effects of noise, you may want to specify a narrower IF bandwidth.

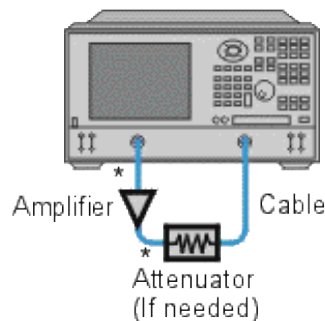

* Direct Connection

7. Remove the amplifier and perform a thru-response calibration. Be sure to include the attenuator and cables in the calibration setup if they will be used when measuring the amplifier.
8. Save the instrument-state to memory.
9. Reconnect the amplifier.
10. Position a marker at approximately mid-span.
11. Adjust the analyzer's scale to 1 dB per division.
12. Store the trace in memory and display Data/Mem.
13. Gradually increase the source power until a 1-dB decrease in gain is observed at the first frequency over some portion of the trace.
14. Use markers to locate the frequency where the 1-dB decrease in gain first occurs. Note this frequency for use in the following measurement.
15. Print the data or save it to a disk.

Swept-Power Gain Compression Measurement

A swept-power gain compression measurement shows the input power resulting in a 1-dB drop in gain as a power ramp at a particular frequency (found in step 13 of the previous measurement) is applied to the amplifier.

1. If not already done, perform the previous measurement of swept-frequency gain compression.
2. Setup an S_{21} measurement in the power-sweep mode. Include the following settings:
 - Set the CW frequency to the frequency noted in step 14 of the previous measurement of swept-frequency gain compression.
 - Enter the start and stop power levels for the sweep. The start power should be in the linear region of the amplifier's response (typically 10 dB below the 1-dB compression point). The stop power should be in the compression region of the amplifier's response.
3. Adjust the scale to 1-dB per division.
4. Use markers (including reference marker) to find the input power where the 1-dB decrease in gain occurs.
5. Print the data or save it to a disk.

Absolute Output Power Measurement

An absolute-power measurement shows the absolute power-out (in dBm) of the amplifier at compression.

1. Select an unratiod (absolute) power measurement. Choose the B input if using the test setup in the previous graphic.
2. Retain the CW frequency used in the previous measurement of swept-power gain compression.
3. Set a marker to the input power level where the 1-dB decrease in gain occurs (found in step 4 of the previous measurement).
4. Scale the displayed measurement for optimum viewing.
5. Read the marker value to find the absolute output power of the amplifier (in dBm) where the 1-dB decrease in gain occurs.
6. Print the data or save it to a disk.

Note: The measurement calibration does not apply to absolute power. Therefore, if there is any attenuation external to the analyzer, you will have to correct for it manually.

Reverse Isolation

Reverse isolation is a measure of amplifier reverse transmission response- from output to input.

[What is Reverse Isolation](#)

[Why Measure Reverse Isolation?](#)

[Accuracy Considerations](#)

[How to Measure Reverse Isolation](#)

[See other Tutorials](#)

What is Reverse Isolation?

Reverse isolation is a measure of how well a signal applied to the device output is "isolated" from its input.

The measurement of reverse isolation is similar to that of forward gain, except:

- The stimulus signal is applied to the amplifier's output port.
- The response is measured at the amplifier's input port.

The equivalent S-parameter is S12.

Why Measure Reverse Isolation?

An ideal amplifier would have infinite reverse isolation-no signal would be transmitted from the output back to the input. However, reflected signals can pass through the amplifier in the reverse direction. This unwanted reverse transmission can cause the reflected signals to interfere with the desired fundamental signal flowing in the forward direction. Therefore, reverse isolation is important to quantify.

Accuracy Considerations

Since amplifiers often exhibit high loss in the reverse direction, generally there is no need for any attenuation that may have been used to protect the port 2 receiver during forward transmission measurements. Removing the attenuation will:

- Increase the dynamic range, resulting in improved measurement accuracy.
- Require a new calibration for maximum accuracy.

The RF source power can be increased to provide more dynamic range and accuracy.

Note: With the attenuation removed and the RF source power increased, a forward sweep could damage the analyzer's port 2 receiver. Do not perform a forward sweep or use 2-port calibration unless the forward power is set low enough to avoid causing port 2 receiver compression or damage.

If the isolation of the amplifier under test is very large, the transmitted signal level may be near the noise floor or crosstalk level of the receiver. To lower the noise floor:

- Use or increase measurement averages.


- Reduce the IF bandwidth of the analyzer.

Note: Reducing IF bandwidth or using averaging improves measurement dynamic range and accuracy, at the expense of reduced measurement speed.

- When crosstalk levels affect the measurement accuracy, reduce the crosstalk error term by performing a response and isolation calibration. When performing the isolation part of the calibration it is important to use the same average factor and IF bandwidth during the calibration and measurement.
- The frequency response of the test setup is the dominant error in a reverse isolation measurement. Performing a thru-response measurement calibration significantly reduces this error. This calibration can be done as part of the response and isolation calibration.
- The amplifier may respond very differently at various temperatures. The tests should be done when the amplifier is at the desired operating temperature.

How to Measure Reverse Isolation

1. Connect the amplifier as shown in the following graphic.

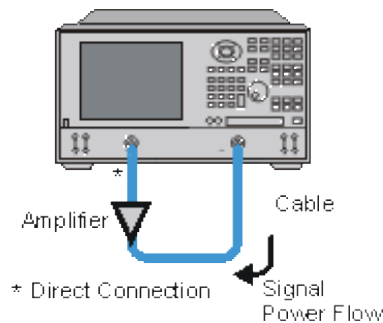

2. Preset the analyzer.
3. Select an S12 measurement.
4. Select the settings for your amplifier under test.
5. Remove the amplifier and perform a thru-response calibration or a response and isolation calibration.
6. Scale the displayed measurement for optimum viewing and use a marker to measure the reverse isolation at a desired frequency.
7. Print or save the data to a disk.

Absolute Output Power

An absolute output-power measurement displays absolute power versus frequency.

[What is Absolute Output Power?](#)

[Why Measure Absolute Output Power?](#)

[Accuracy Considerations](#)

[How to Measure Absolute Output Power](#)

[See other Amplifier Parameters topics](#)

What is Absolute Output Power?

An absolute-output power measurement displays the power present at the analyzer's input port. This power is absolute-it is not referenced (ratioed) to the incident or source power. In the log mag format, values associated with the grid's vertical axis are in units of dBm, which is the power measured in reference to 1 mW.

- 0 dBm = 1 mW
- -10 dBm = 100 μ W
- +10 dBm = 10 mW

In the linear mag format, values associated with the grid's vertical axis are in units of watts (W).

Why Measure Absolute Output Power?

Absolute output power is measured when the amplifier's output must be quantified as absolute power rather than a ratioed relative power measurement. For example, during a gain compression measurement, it is typical to also measure absolute output power. This shows the absolute power out of the amplifier where 1-dB compression occurs.

Accuracy Considerations

The output power of the amplifier should be sufficiently attenuated if necessary. Too much output power could:

- Damage the analyzer receiver
- Exceed the input compression level of the analyzer receiver, resulting in inaccurate measurements.

Attenuation of the amplifier's output power can be accomplished using either attenuators or couplers


The amplifier may respond very differently at various temperatures. The tests should be done when the amplifier is at the desired operating temperature.

How to Measure Absolute Power

Do the following to measure absolute output power:

1. Preset the analyzer.


2. Select an unratiod power measurement (receiver B).
3. Set the analyzer's source power to 0 dBm.
4. Select an external attenuator (if needed) so the amplifier's output power will be sufficiently attenuated to avoid causing receiver compression or damage to the analyzer's port-2.
5. Connect the amplifier as shown in the following graphic, and provide the dc bias.

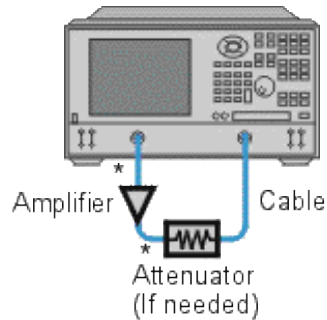

* Direct Connection

6. Select the analyzer settings for your amplifier under test.
7. Remove the amplifier and connect the measurement ports together. Store the data to memory. Be sure to include the attenuator and cables in the test setup if they will be used when measuring the amplifier.
8. Save the instrument state to memory.
9. Reconnect the amplifier.
10. Select the data math function Data/Memory.
11. Scale the displayed measurement for optimum viewing and use a marker to measure the absolute output-power at a desired frequency.
12. Print or save the data to a disk.

PNA Object Model

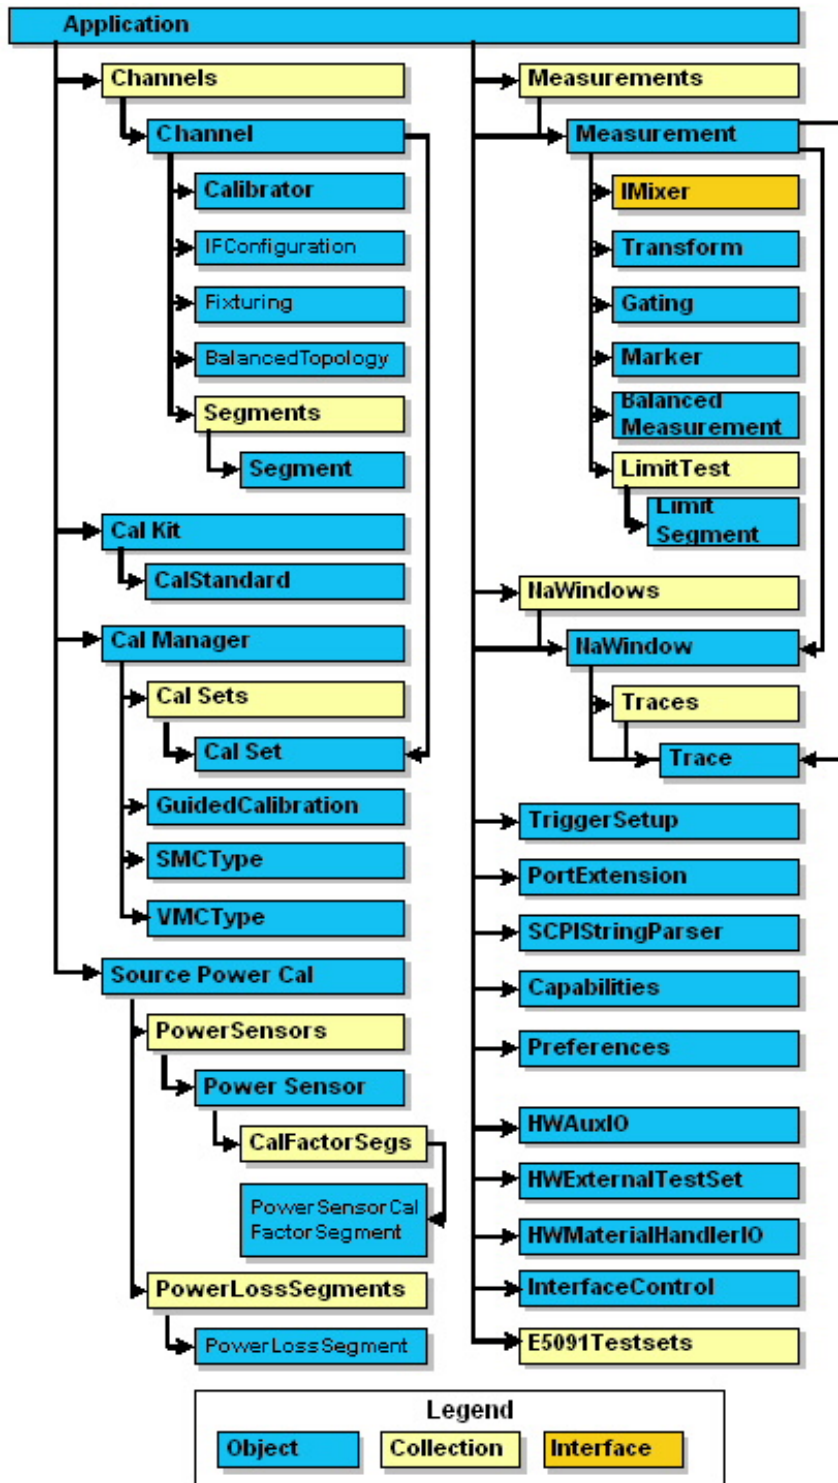

- See a list of obsolete commands.

Application Object

Description

The Application object is the highest object in the PNA [object model](#). This object presents methods and properties that affect the entire analyzer, rather than a specific channel or measurement. For example, the application object provides the GetIDString method. There's only one ID string for the instrument, unrelated to the channel or parameter being measured. Likewise, the TriggerSignal Property is global to the instrument. You can elect to use an internally generated (free run) trigger or a manual trigger. Either way, that type of trigger generation will be used on all measurements, on all channels. Therefore, it is under the Application object.

Accessing the Application object

This object is unique in that you must **create** this object rather than just get a handle to it.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)
```

Replace <analyzerName> with the full computer name of your PNA. For example, "My PNA". See [Change Computer Name](#).


See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Getting a Handle to an Object](#).

(**Bold** Methods or Properties provide access to a child object)

Methods	Interface	Description
	See History	
ActivateWindow	IApplication	Makes a window object the Active Window.
AllowAllEvents	IApplication	Monitors all events
 AllowEventCategory	IApplication	Monitors an event category
AllowEventMessage	IApplication	Monitors an event
AllowEventSeverity	IApplication	Monitors an event severity level
BuildHybridKit	IApplication	Defines the user kit as port1kit + port2kit.
Channel	IApplication	Stimulus values like frequency, power, IF bandwidth, and number of points.
CreateCustomMeasurementEx	IApplication3	Creates a new custom measurement with initialization.
CreateCustomMeasurement	IApplication	OBSOLETE - CreateCustomMeasurementEx Method
CreateMeasurement	IApplication	Creates a new measurement.
CreateSParameter	IApplication	OBSOLETE - Use Create SParameterEX Method

<u>CreateSParameterEx</u>	IApplication	Creates a new S-Parameter measurement with a 3-port load.
<u>DeleteShortcut</u>	IApplication	Removes a macro (shortcut) from the list of macros
<u>DisallowAllEvents</u>	IApplication	Monitors NO events
<u>DoPrint</u>	IApplication	Prints the screen to the active Printer.
<u>ExecuteShortcut</u>	IApplication	Executes a macro (shortcut) stored in the analyzer.
<u>GetAuxIO</u>	IApplication	Returns a handle to the AuxIO interface
<u>GetCalManager</u>	IApplication	Returns a handle to the CalManager interface
<u>GetExternalTestSetIO</u>	IApplication	Returns a handle to the ExternalTestSet IO interface
<u>GetMaterialHandlerIO</u>	IApplication	Returns a handle to the MaterialHandlerIO interface
<u>GetShortcut</u>	IApplication	Returns the title and path of the specified macro (shortcut).
<u>LaunchCalWizard</u>	IApplication	Launches the Cal Wizard
<u>ManualTrigger</u>	IApplication	Triggers the analyzer when TriggerSignal = naTriggerManual.
<u>Preset</u>	IApplication	Resets the analyzer to factory defined default settings.
<u>PrintToFile</u>	IApplication	Saves the screen data to bitmap (.bmp) file of the screen.
<u>PutShortcut</u>	IApplication	Puts a Macro (shortcut) file into the analyzer.
<u>Quit</u>	IApplication	Ends the Network Analyzer application.
<u>Recall</u>	IApplication	Recalls a measurement state, calibration state, or both from the hard drive into the analyzer.
<u>RecallKits</u>	IApplication	Recalls the calibration kits definitions that were stored with the SaveKits command.
<u>Reset</u>	IApplication	Removes all existing windows and measurements.
<u>RestoreCalKitDefaults</u>	IApplication	Restores the factory defaults for the specified kit.
<u>RestoreCalKitDefaultsAll</u>	IApplication	Restores the factory defaults for all kits.
<u>Save</u>	IApplication	Saves files to disk
<u>SaveCitiDataData</u>	IApplication4	Saves UNFORMATTED trace data to .cti file.
<u>SaveCitiFormattedData</u>	IApplication4	Saves FORMATTED trace data to .cti file.
<u>SaveKits</u>	IApplication	Saves all cal kits to disk.
<u>SetFailOnOverRange</u>	IApplication	Causes over range values to return an error code
<u>ShowStatusBar</u>	IApplication	Shows and Hides the Status Bar.

<u>ShowStimulus</u>	IApplication	Shows and Hides Stimulus information.
<u>ShowTitleBars</u>	IApplication	Shows and Hides the Title Bars.
<u>ShowToolBar</u>	IApplication	Shows and Hides the specified Toolbar.
<u>UserPreset</u>	IApplication7	Performs a User Preset.
<u>UserPresetLoadFile</u>	IApplication7	Loads an existing instrument state file (.sta or .cst) to be used for User Preset.
<u>UserPresetSaveState</u>	IApplication7	Saves the current instrument settings as UserPreset.sta.

Properties

Description

<u>ActiveCalKit</u>	IApplication	Returns a pointer to the kit identified by kitNumber.
<u>ActiveChannel</u>	IApplication	Returns a handle to the Active Channel object.
<u>ActiveMeasurement</u>	IApplication	Returns a handle to the Active Measurement object.
<u>ActiveNAWindow</u>	IApplication	Returns a handle to the Active Window object.
<u>ArrangeWindows</u>	IApplication	Sets or returns the arrangement of all the windows.
<u>CalKitType</u>	IApplication	Sets or returns the calibration kit type for to be used for calibration or for kit modification. Shared with the CalKit object.
<u>Capabilities</u>	IApplication4	Return capabilities of the remote PNA.
<u>Channels</u>	IApplication	Collection for iterating through the channels
<u>CoupledMarkers</u>	IApplication	Sets (or reads) coupled markers ON and OFF
<u>DisplayAutomationErrors</u>	IApplication2	Enables or disables automation error messages from being displayed on the screen. U
<u>DisplayGlobalPassFail</u>	IApplication6	Shows or hides the dialog which displays global pass/fail results.
<u>E5091Testsets</u>	IApplication8	Collection to control the E5091A testset.
<u>ExternalALC</u>	IApplication	Sets or returns the source of the analyzer leveling control.
<u> GPIBAddress</u>	IApplication8	Sets and returns the PNA GPIB address.
<u> GPIBMode</u>	IApplication	Makes the analyzer the system controller or a talker/listener.
<u>IDString</u>	IApplication	Returns the model, serial number and software revision of the analyzer
<u>InterfaceControl</u>	IApplication8	Control the Interface control features.
<u>LocalLockoutState</u>	IApplication4	Prevents use of the mouse, keyboard, and front panel while your program is running.

<u>Measurements</u>	IApplication	Collection for iterating through the Application measurements.
<u>MessageText</u>	IApplication	Returns text for the specified eventID
<u>NaWindows</u>	IApplication	Collection for iterating through the Application windows.
<u>NumberOfPorts</u>	IApplication	Returns the number of hardware source ports on the PNA
<u>Options</u>	IApplication	Returns the options on the analyzer
<u>Port Extensions</u>	IApplication	Obsolete Use <u>Fixturing Object</u>
<u>Preferences</u>	IApplication5	Preferences for saving citifiles.
<u>ScpiStringParser</u>	IApplication	Provides the ability to send a SCPI command from within the COM command.
<u>SecurityLevel</u>	IApplication4	Turns ON or OFF the display of frequency information.
<u>SICL</u>	IApplication5	Allows control of the PNA via SICL
<u>SICLAddress</u>	IApplication8	Sets and returns the PNA SICL address
<u>SourcePowerCalibrator</u>	IApplication2	Allows capability for performing source power calibrations.
<u>SourcePowerState</u>	IApplication	Turns Source Power ON and OFF.
<u>SystemImpedanceZ0</u>	IApplication	Sets the analyzer impedance value.
<u>SystemName</u>	IApplication	Returns the full computer name of the PNA.
<u>TriggerDelay</u>	IApplication	Sets or returns the delay time for a trigger.
<u>TriggerSetup</u>	IApplication4	Controls triggering for the entire PNA application.
<u>TriggerSignal</u>	IApplication	Obsolete - use <u>Source Property</u>
<u>TriggerType</u>	IApplication	Obsolete - use <u>Scope Property</u>
<u>UserPresetEnable</u>	IApplication7	'Checks' and 'clears' the enable box on the User Preset dialog box.
<u>VelocityFactor</u>	IApplication	Sets the velocity factor to be used with Electrical Delay, Port Extensions, and Time Domain marker distance calculations.
<u>Visible</u>	IApplication	Makes the Network Analyzer application visible or not visible.
<u>WindowState</u>	IApplication	Sets or returns the window setting of Maximized, Minimized, or Normal. Shared with the NAWindow Object

Events	Interface	Description
--------	-----------	-------------

<u>OnCalEvent</u>	IApplication	Triggered by a calibration event.
<u>OnChannelEvent</u>	IApplication	Triggered by a channel event.
<u>OnDisplayEvent</u>	IApplication	Triggered by a display event.
<u>OnHardwareEvent</u>	IApplication	Triggered by a hardware event.
<u>OnMeasurementEvent</u>	IApplication	Triggered by a measurement event.
<u>OnSCPIEvent</u>	IApplication	Triggered by a SCPI event.
<u>OnSystemEvent</u>	IApplication	Triggered by a system event.
<u>OnUserEvent</u>	IApplication	For future use

IApplication History

Interface	Introduced with PNA Rev:
IApplication	1.0
IApplication2	3.0
IApplication3	3.2
IApplication4	3.5
IApplication5	4.0
IApplication6	5.0
IApplication7	5.0
IApplication8	5.2

BalancedMeasurement Object

Description

These properties set the measurement type that is used with balanced topologies.

Use the [BalancedTopology Object](#) to set the topology and port mappings for the DUT,

Accessing the BalancedMeasurement object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim balMeas As BalancedMeasurement
Set balMeas = app.ActiveMeasurement.BalancedMeasurement
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[About Balanced Measurements](#)

(**Bold** Methods or Properties provide access to a child object)


Method	Description
--------	-------------

None

Property	Interface	Description
----------	-----------	-------------

[See History](#)

[BalancedMode](#) IBalancedMeasurement Sets and returns whether the balanced transform is ON or OFF.

 [BalancedTopology](#) IBalancedMeasurement Sets and returns the topology of a balanced DUT.

[BBalMeasurement](#) IBalancedMeasurement Sets and returns the measurement for the Balanced - Balanced topology.

[SBalMeasurement](#) IBalancedMeasurement Sets and returns the measurement for the Single-Ended - Balanced topology.

[SSBMeasurement](#) IBalancedMeasurement Sets and returns the measurement for the Single-Ended - Single-Ended - Balanced topology

IBalancedMeasurement History

Interface	Introduced with PNA Rev:
IBalancedMeasurement	5.0

BalancedTopology Object

Description

The [DUTTopology](#) property sets and returns the topology of a balanced DUT.

The following methods **set** the port mappings for the DUT.

The remaining properties **return** the port mappings for the DUT.

Use the [BalancedMeasurement](#) object to set the measurement type.

Accessing the BalancedTopology object

```
Dim app as AgilentPNA835x.Application
Dim chan as Channel
Set chan = app.ActiveChannel


Dim balTopology as BalancedTopology
Set balTopology = chan.BalancedTopology
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[About Balanced Measurements](#)

Method	Interface	Description
	See History	
SetBBPorts	IBalancedTopology	Sets the physical port mappings for the Balanced - Balanced DUT topology.
SetSBPorts	IBalancedTopology	Sets the physical port mappings for the Single-Ended - Balanced DUT topology.
 SetSSBPorts	IBalancedTopology	Sets the physical port mappings for the Single-Ended - Single-Ended - Balanced DUT topology.

Property	Interface	Description
BB_BalPort1Negative	IBalancedTopology	Returns the PNA port number that is connected to the Negative side of the DUT's logical Port 1 .
BB_BalPort1Positive	IBalancedTopology	Returns the first positive balanced port number in the Balanced - Balanced topology
BB_BalPort2Negative	IBalancedTopology	Returns the second negative balanced port number in the Balanced - Balanced topology.

<u>BB_BalPort2Positive</u>	IBalancedTopology	Returns the second positive balanced port number in the Balanced - Balanced topology.
<u>DUTTopology</u>	IBalancedTopology	Sets and returns the device topology setting.
<u>SB_BalPortNegative</u>	IBalancedTopology	Returns the negative balanced port number in the Single-Ended - Balanced topology.
<u>SB_BalPortPositive</u>	IBalancedTopology	Returns the positive balanced port number in the Single-Ended - Balanced topology.
<u>SB_SEPort</u>	IBalancedTopology	Returns the single ended port number in the Single-Ended - Balanced topology.
<u>SSB_BalPortNegative</u>	IBalancedTopology	Returns the negative balanced port number in the Single-Ended - Single-Ended - Balanced topology.
<u>SSB_BalPortPositive</u>	IBalancedTopology	Returns the positive balanced port number in the Single-Ended - Single-Ended - Balanced topology
<u>SSB_SEPort1</u>	IBalancedTopology	Returns the first single ended port in the Single-Ended - Single-Ended - Balanced topology.
<u>SSB_SEPort2</u>	IBalancedTopology	Returns the second single ended port in the Single-Ended - Single-Ended - Balanced topology.

BalancedTopology History

Interface	Introduced with PNA Rev:
IBalancedTopology	5.0

CalFactorSegments Collection

Description

A collection object that provides a mechanism for iterating through the segments of a power sensor cal factor table.

Accessing the CalFactorSegments collection

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim calFact As CalFactorSegments
Set calFact = app.SourcePowerCalibrator.PowerSensors(1).CalFactorSegments
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Description
Add	Adds a PowerSensorCalFactorSegment object to the collection
Item	Use to get a handle to a PowerSensorCalFactorSegment object in the collection.
Remove	Removes an object from the collection.

Properties	Description
Count	Returns the number of objects in the collection.
Parent	Returns a handle to the Parent object (PowerSensor) of this collection.

Calibrator Object

See [Calibrator Methods and Properties](#)

See [ICalData Interface](#) for putting and getting typed Calibration data.


Description

The Calibrator object, a child of the channel, is used to perform an Unguided calibration.

Note: You can NOT perform a full 3 or 4-port using the Calibrator object; you must use the [GuidedCalibration object](#).

There must be a measurement present for the calibrator to use or you will receive a "no measurement found" error. Therefore, to perform a 2-port cal, you must have any S-parameter measurement on the channel. For a 1-port measurement, you must have the measurement (S11 or S22) on the channel. The same is true for a response measurement.

There are a number of approaches to calibration with the calibrator object:

- You can collect data yourself and download it to the ACQUISITION buffer. The acquisition buffer holds the actual measured data for each standard. See the PNA [data map](#).
 1. Calibrator.[SetCallInfo](#)
 2. Connect a standard
 3. Trigger a sweep
 4. Retrieve the data for the standard
 5. Download the data - calibrator.[putStandard](#)
 6. Repeat for each standard
 7. Calibrator.[CalculateErrorCoefficients](#)
- You can tell the calibrator to acquire a standard. In this case, the calibrator collects the data and places it in the ACQUISITION buffer.
 1.  Calibrator.[SetCallInfo](#)
 2. Connect a standard
 3. Calibrator.[AcquireCalStandard2](#)
 4. Repeat for each standard
 5. Calibrator.[CalculateErrorCoefficients](#)
- You can put previously-retrieved error terms in the error correction buffer.
 1. [PutErrorTerm](#)
 2. Repeat for each term
 3. Measurement.[Caltype](#) = pick one
- You can also "piece together" a 2-port cal from two 1-port cal (S11 and S22) and four response (thru) cal. The system will detect that all the standards needed for a 2-port cal have been acquired even though they may not

have gathered at the same time.

Accessing the Calibrator object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim cal As ICalibrator
Set cal = app.ActiveChannel.Calibrator
```

See Also:

- [PNA Automation Interfaces](#)
- [The PNA Object Model](#)
- [Learn about reading and writing Calibration data.](#)

Methods	Interface	Description
	See History	
AcquireCalConfidenceCheckECAL	ICalibrator	Obsolete - use AcquireCalConfidenceCheckECALEx
AcquireCalConfidenceCheckECALEx	ICalibrator4	Transfers ECAL confidence data into analyzer memory
AcquireCalStandard	ICalibrator	Obsolete - use AcquireCalStandard2
AcquireCalStandard2	ICalibrator	Causes the analyzer to measure a calibration standard. Also provides for sliding load.
CalculateErrorCoefficients	ICalibrator	Generates Error Terms from standard and actual data in the error correction buffer.
DoECAL1Port	ICalibrator	Obsolete - use DoECAL1PortEx
DoECAL1PortEx	ICalibrator4	Completes a 1 port ECAL
DoECAL2Port	ICalibrator	Obsolete - use DoECAL2PortEx
DoECAL2PortEx	ICalibrator4	Completes a 2 port ECAL
DoneCalConfidenceCheckECAL	ICalibrator	Concludes an ECAL confidence check
DoReceiverPowerCal	ICalibrator5	Perform a receiver power cal.
GetECALModuleInfo	ICalibrator	Obsolete - use GetECALModuleInfoEx
GetECALModuleInfoEx	ICalibrator4	Returns information about the attached module
getErrorTerm	ICalibrator	Obsolete - replaced by GetErrorTermByString
getStandard	ICalibrator	Obsolete - replaced by GetStandardByString

<u>putErrorTerm</u>	ICalibrator	Obsolete - replaced by <u>PutErrorTermByString</u>
<u>putStandard</u>	ICalibrator	Obsolete - replaced by <u>PutStandardByString</u>
<u>SaveCalSets</u>	ICalibrator	Writes new or changed Cal Sets to disk. Shared with the CalManager Object
<u>setCallInfo</u>	ICalibrator	Specifies the type of calibration and prepares the internal state for the rest of the calibration.
Properties	Interface	Description
<u>AcquisitionDirection</u>	ICalibrator	Specifies the direction in a 2-Port cal using one set of standards.
<u>ECALCharacterization</u>	ICalibrator2	Obsolete - use ECALCharacterizationEx
<u>ECALCharacterizationEx</u>	ICalibrator4	Specifies which set of characterization data within an ECal module will be used for ECal operations with that module.
<u>ECAL Isolation</u>	ICalibrator	Obsolete - No replacement
<u>ECALPortMap</u>	ICalibrator3	Obsolete - use ECALPortMapEx
<u>ECALPortMapEx</u>	ICalibrator4	Specifies which ports of the ECal module are connected to which ports of the PNA.
<u>IsECALModuleFound</u>	ICalibrator	Obsolete - use IsECALModuleFoundEx
<u>IsECALModuleFoundEx</u>	ICalibrator4	Tests communication between the PNA and ECAL Module
<u>OrientECALModule</u>	ICalibrator3	Specifies if the PNA should perform orientation of the ECal module during calibration.
<u>Simultaneous2PortAcquisition</u>	ICalibrator	Allows the use of 2 sets of standards at the same time.

ICalibrator History

Interface	Introduced with PNA Rev:
ICalibrator	1.0
ICalibrator2	3.1
ICalibrator3	3.1
ICalibrator4	3.5
ICalibrator5	5.0

ICalData Interface

Description

Contains methods for putting Calibration data in and getting Calibration data out of the analyzer using typed data. This interface transfers data more efficiently than variant data.

There is also an [ICalData Interface](#) on the CalSet Object

[Learn about reading and writing Calibration data.](#)

Methods	Description
getErrorTermComplex	Retrieves error term data
getStandardComplex	Retrieves calibration data from the acquisition data buffer (before error-terms are applied).
putErrorTermComplex	Puts error term data
putStandardComplex	Puts calibration data into the acquisition data buffer (before error-terms are applied).

Properties	Description
------------	-------------

None

ICalData History

Interface	Introduced with PNA Rev:
ICalData	1.0

CalKit Object

Description

The calkit object provides the properties and methods to access and modify a calibration kit. The calkitType property can be set from two objects:

- Application object - app.calKitType
- CalKit object - calKit.calKitType

Both of these commands specify or read the calibration kit type. When specified, the cal kit also becomes the Active cal kit.

Accessing a CalKit object

To get a handle to a cal kit, use **app.ActiveCalKit**.

The calKit object behaves differently from other objects in the system in that you can only have a handle to **one** cal kit -- the active calkit. Therefore, when you change the calkitType from either the Application object or the CalKit object, you may also be changing the object to which you may have other references.

For example, the following example specifies two calKit type objects and in turn, assigns them to two different variables: ck1 and ck2.

```
Dim app As AgilentPNA835x.Application
Dim ck1 As calKit
Dim ck2 As calKit

Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)
app.CalKitType = naCalKit_User1
Set ck1 = app.ActiveCalKit
ck1.Name = "My CalKit1"

app.CalKitType = naCalKit_User2
Set ck2 = app.ActiveCalKit
ck2.Name = "My CalKit2"

Print "ck1: " & ck1.Name
Print "ck2: " & ck2.Name
```

When the pointer to each of these kits is read (printed), they each have a pointer to the last kit to be assigned to the Active cal kit:

```
ck1: My CalKit2
ck2: My CalKit2
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

(**Bold** Methods or Properties provide access to a child object)

Methods	Description
<u>getCalStandard</u>	Returns a handle to a calibration standard for modifying its definitions.
<u>GetStandardsForClass</u>	Returns the calibration standard numbers for a specified calibration class.
<u>SetStandardsForClass</u>	Sets the calibration standard numbers for a specified calibration class

Properties	Description
<u>CalKitType</u>	Sets or returns the calibration kit type for to be used for calibration or for kit modification. Shared with the Application object.
<u>Name</u>	Sets and returns the name of the cal kit
<u>PortLabel</u>	Labels the ports for the kit; only affects the cal wizard annotation.
<u>StandardForClass</u>	Obsolete Use <u>GetStandardForClass</u> and <u>SetStandardForClass</u> . Maps a standard device to a cal class.

ICalKit History

Interface	Introduced with PNA Rev:
ICalKit	1.0

CalManager Object

Description

Use this interface to list, save, and delete Cal Sets.

Accessing the CalManager object

Get a handle to a the CalManager with the app.[GetCalManager](#) Method.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim mgr as ICalManager
Set mgr = app.GetCalManager
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

(**Bold** Methods or Properties provide access to a child object)

Methods	Interface	Description
CreateCalSet	ICalManager	Creates a new Cal Set
CreateCustomCal	ICalManager2	Creates a custom cal object.
DeleteCalSet	ICalManager	Deletes a Cal Set
GetCalSetByGUID	ICalManager	Get a handle to a Cal Set
GetCalSetCatalog	ICalManager	Gets a list of Cal Sets
GetCalSetUsageInfo	ICalManager	Returns the Cal Set ID and Error Term ID currently in use
GetCalTypes	ICalManager2	Query for a list of available calibration types.
GetRequiredEtermNames	ICalManager2	Returns an array of strings specifying the error terms required by the Cal Type correction algorithm.
SaveCalSets	ICalManager	Writes new or changed Cal Sets to disk Shared with the Calibrator Object

Properties

Cal Sets	ICalManager	Collection for iterating through all the Cal Sets in the analyzer.
---------------------------------	-------------	--

GuidedCalibration

ICalManager4 Used to perform a Guided Calibration.

ICalManager History

Interface	Introduced with PNA Rev:
ICalManager	2.0
CalManager2	3.1
CalManager3	3.5
CalManager4	5.0

CalSet Object

See [ICalData Interface](#) for putting and getting typed Cal Set data.

Description

Use this interface to query and or change the contents of a Cal Set.

Accessing the CalSet object

Get a handle to a CalSet object by using the CalSets collection. This is done through the CalManager object with the [app.GetCalManager](#) Method.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim calst As ICalSet
Set calst = app.GetCalManager.CalSets.Item(1)
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Reading and Writing Calibration data.](#)

Methods	Interface	Description
	See History	
CloseCalSet	ICalSet	Obsolete - No longer necessary.
ComputeErrorTerms	ICalSet	Computes error terms for the CalType specified by a preceding OpenCal Set call.
Copy	ICalSet	Creates a new Cal Set and copies the current Cal Set data into it.
GetErrorTerm	ICalSet	Obsolete - Use getErrorTermByString
getErrorTermByString	ICalSet2	Returns variant error term data by specifying the string name of the error term.
getErrorTermList	ICalSet	Obsolete - Use getErrorTermList2
getErrorTermList2	ICalSet2	Returns a list of error term names found in a calset.
GetGUID	ICalSet	Returns the GUID identifying a Cal Set
getStandard	ICalSet	Obsolete - Use getStandardByString
getStandardByString	ICalSet2	Returns variant standard acquisition data by specifying the string name of the standard.
getStandardsList	ICalSet	Obsolete - Use getStandardList2

<u>getStandardList2</u>	ICalSet2	Returns a list of standard names found in a Cal Set.
<u>HasCalType</u>	ICalSet	Verifies that the Cal Set object contains the error terms required to apply the specified CalType to an appropriate measurement.
<u>OpenCalSet</u>	ICalSet	Obsolete - No longer necessary.
<u>putErrorTerm</u>	ICalSet	Obsolete - Use <u>putErrorTermByString</u>
<u>putErrorTermByString</u>	ICalSet2	Writes variant error term data by specifying the string name of the error term.
<u>putStandard</u>	ICalSet	Obsolete - Use <u>putStandardByString</u>
<u>putStandardByString</u>	ICalSet2	Writes variant standard acquisition data by specifying the string name of the standard.
<u>Save</u>	ICalSet	Saves the current Cal Set to disk.
<u>StringToNACalClass</u>	ICalSet	Converts string values from GetStandardsList into enumeration data
<u>StringToNAErrorTerm2</u>	ICalSet	Converts string values from GetErrorTermList into enumeration data

Properties	Description
------------	-------------

<u>AlternateSweep</u>	ICalSet3	Reads sweep either alternate or chopped.
<u>Attenuator</u>	ICalSet3	Returns the value of the attenuator control for the specified port number.
<u>AttenuatorMode</u>	ICalSet3	Returns the mode of operation (auto or manual) of the attenuator control for the specified port number.
<u>CouplePorts</u>	ICalSet3	Returns state of couple ports (ON or OFF)
<u>CWFrequency</u>	ICalSet3	Returns CW Frequency
<u>Description</u>	ICalSet	Set or return the descriptive string assigned to the Cal Set
<u>DwellTime</u>	ICalSet3	Returns the dwell time for the channel.
<u>FrequencyOffsetCWOverride</u>	ICalSet3	Reads state of CW Override (ON or OFF)
<u>FrequencyOffsetDivisor</u>	ICalSet3	Reads Frequency Offset Divisor value
<u>FrequencyOffsetFrequency</u>	ICalSet3	Reads Offset Frequency
<u>FrequencyOffsetMultiplier</u>	ICalSet3	Reads Frequency Offset Multiplier value
<u>FrequencyOffsetState</u>	ICalSet3	Reads Frequency Offset state (ON or OFF)
<u>IFBandwidth</u>	ICalSet3	Reads IF Bandwidth of the channel

<u>LastModified</u>	ICalSet3	Reads the time stamp of when the file was last modified
<u>NumberOfPoints</u>	ICalSet3	Returns the Number of Points of the channel.
<u>PowerSlope</u>	ICalSet3	Returns the Power Slope value.
<u>ReceiverAttenuator</u>	ICalSet3	Returns the value of the specified receiver attenuator control.
<u>StartFrequency</u>	ICalSet3	Returns the start frequency of the channel.
<u>StartPower</u>	ICalSet3	Returns the start power of the PNA when sweep type is set to Power Sweep.
<u>StimulusValues</u>	ICalSet3	Returns x-axis values for stimulus or response frequencies
<u>StopFrequency</u>	ICalSet3	Returns the stop frequency of the channel.
<u>StopPower</u>	ICalSet3	Returns the stop power of the PNA when sweep type is set to Power Sweep.
<u>SweepGenerationMode</u>	ICalSet3	Returns the method being used to generate a sweep: analog or stepped.
<u>SweepTime</u>	ICalSet3	Returns the sweep time of the analyzer.
<u>SweepType</u>	ICalSet3	Returns the type of X-axis sweep that is performed on a channel.
<u>TestPortPower</u>	ICalSet3	Returns the RF power level for the channel.

ICalSet History

Interface	Introduced with PNA Rev:
ICalSet	2.0
ICalSet2	3.0
ICalSet3	3.2

ICalData Interface

Description

Use this interface as an alternative to the ICalSet Interface to avoid using variants when transmitting data to and from the Cal Set

[Learn about reading and writing Calibration data.](#)

Methods	Interface	Description
	<u>See History</u>	
<u>getErrorTermComplex</u>	ICalData2	Obsolete - Use <u>getErrorTermComplexByString</u>
<u>getErrorTermComplexByString</u>	ICalData3	Returns typed error term data by specifying the string name of the error term.
<u>getStandardComplex</u>	ICalData2	Obsolete - Use <u>getStandardComplexByString</u>
<u>getStandardComplexByString</u>	ICalData3	Returns typed standard acquisition data by specifying the string name of the standard.
<u>putErrorTermComplex</u>	ICalData2	Obsolete - Use <u>putErrorTermComplexByString</u>
<u>putErrorTermComplexByString</u>	ICalData3	Writes typed error term data by specifying the string name of the error term.
<u>putStandardComplex</u>	ICalData2	Obsolete - Use <u>putStandardComplexByString</u>
<u>putStandardComplexByString</u>	ICalData3	Writes typed standard acquisition data by specifying the string name of the standard.

Properties	Description
------------	-------------

None

History

Interface	Introduced with PNA Rev:
-----------	--------------------------

The original ICalData Interface was introduced with PNA 1.0 on the Calibrator Object.

ICalData2	2.0
-----------	-----

ICalData3	3.1
-----------	-----

Cal Sets Collection

Description

A collection object that provides a mechanism for iterating through all the Cal Sets in the analyzer. There is no ordering to the items in the collection. Therefore make no assumptions about the formatting of the collection.

Accessing the CalSets collection

Get a handle to the CalSets collection through the CalManager object with the `app.GetCalManager` Method.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim calsts As CalSets
Set calsts = app.GetCalManager.CalSets
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Description
Item	Returns a handle to a Cal Set object in the collection.
Remove	Deletes the Cal Set residing at position index in the collection.

Properties	Description
Count	Returns the number of Cal Sets in the collection.

CalStandard Object

Description

Contains all of the settings that are required to modify a calibration standard.

Accessing the CalStandard object

Get a handle to a standard with the `calkit.GetCalStandard` Method.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim std As ICalStandard
Set std = app.ActiveCalKit.GetCalStandard(1)
std.Delay = 0.00000003
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Reading and Writing Calibration data.](#)

Methods

None

Properties	Interface	Description
	See History	
C0	ICalStandard	Sets and Returns the C0 (C-zero) value (the first capacitance value) for the calibration standard, when the Type is set to "naOpen".
C1	ICalStandard	Sets and Returns the C1 value (the second capacitance value) for the calibration standard, when the Type is set to "naOpen".
C2	ICalStandard	Sets and Returns the C2 value (the third capacitance value) for the calibration standard, when the Type is set to "naOpen".
C3	ICalStandard	Sets and Returns the C3 value (the fourth capacitance value) for the calibration standard, when the Type is set to "naOpen".
Delay	ICalStandard	Sets and Returns the electrical delay value for the calibration standard.
L0	ICalStandard	Sets and Returns the L0 (L-zero) value (the first inductance value) for the calibration standard, when the Type is set to "naShort".
L1	ICalStandard	Sets and Returns the L1 value (the second inductance value) for the calibration standard, when the Type is set to "naShort"..
L2	ICalStandard	Sets and Returns the L2 value (the third inductance value) for the calibration standard, when the Type is set to "naShort"..

<u>L3</u>	ICalStandard	Sets and Returns the L3 value (the third inductance value) for the calibration standard, when the Type is set to "naShort"..
<u>Label</u>	ICalStandard	Sets and Returns the label for the calibration standard.
<u>loss</u>	ICalStandard	Sets and Returns the insertion loss for the calibration standard.
<u>Maximum Frequency</u>	ICalStandard	Sets and Returns the maximum frequency for the calibration standard.
<u>Medium</u>	ICalStandard	Sets and Returns the media type of the calibration standard.
<u>Minimum Frequency</u>	ICalStandard	Sets and Returns the minumum frequency for the calibration standard.
<u>Type</u>	ICalStandard	Sets and Returns the type of calibration standard. Selections are: naOpen, naShort, naLoad, naThru, naArbitraryImpedance and naSliding.
<u>TZReal</u>	ICalStandard2	Sets and Returns the TZReal value (the Real Terminal Impedance value) for the calibration standard, when the Type is set to "naArbitraryImpedance".
<u>TZImag</u>	ICalStandard2	Sets and Returns the TZImag value (the Imaginary Terminal Impedance value) for the calibration standard, when the Type is set to "naArbitraryImpedance".
<u>Z0</u>	ICalStandard	Sets and Returns the characteristic impedance for the calibration standard.

ICalStandard History

Interface	Introduced with PNA Rev:
CalStandard	1.0
CalStandard2	3.0

Capabilities Object

Description

These properties return capabilities of the remote PNA.

Accessing the Capabilities object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim cap As Capabilities
Set cap = app.Capabilities
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[ICapabilities History](#)

Methods

None

Properties	Description
FirmwareMajorRevision	Returns integer portion of firmware revision number.
FirmwareMinorRevision	Return decimal portion of firmware revision number.
FirmwareSeries	Returns the Alpha portion of the firmware revision number.
InternalTestsetPortCount	Returns the number of test ports (2 or 3).
IsFrequencyOffsetPresent	Returns the presence of Frequency Offset Option 080 (True or False).
IsReceiverStepAttenuatorPresent	Returns the presence of receiver step attenuators (True or False).
IsReferenceBypassSwitchPresent	Returns the presence of the reference switch (True or False).
MaximumFrequency	Returns the maximum frequency of the PNA.
MaximumNumberOfPoints	Returns the maximum possible number of data points.
MaximumReceiverStepAttenuator	Returns the maximum amount of receiver attenuation.
MaximumSourceALCPower	Returns the maximum amount of source ALC power.
MaximumSourceStepAttenuator	Returns the maximum amount of source attenuation.
MinimumFrequency	Returns the minimum frequency of the PNA.

<u>MinimumNumberOfPoints</u>	Returns the minimum possible number of data points.
<u>MinimumReceiverStepAttenuator</u>	Returns the minimum amount of receiver attenuation.
<u>MinimumSourceALCPower</u>	Returns the minimum amount of source ALC power.
<u>ReceiverCount</u>	Returns the number of receivers in the PNA.
<u>ReceiverStepAttenuatorStepSize</u>	Returns the step size of the attenuator.
<u>SourceCount</u>	Returns the number of sources.

ICapabilities History

I Interface	Introduced with PNA Rev:
ICapabilities	3.5

Channel Object

See [SourcePowerCalData Interface](#) for putting and getting typed source power calibration data.

Description

The channel object is like the engine that produces data. Channel settings consist of stimulus values like frequency, power, IF bandwidth, and number of points.

Accessing the Channel object

You can get a handle to a channel in a number of ways. But first you have to make sure that the channel exists. When you first startup the analyzer, there is one S11 measurement on channel 1. Thus there is only one channel in existence. You can do the following:

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim chan As IChannel
Set chan = app.ActiveChannel
```

or

```
Set chan = app.Channels(2)
```

The first method returns the channel object that is driving the active measurement. If there is no measurement, there may not be a channel. Once a channel is created, it does not go away. So if there once was a measurement (hence a channel), the channel will still be available.

If there is no channel you can create one in a couple ways. You can do the following:

```
Pna.CreateMeasurement( ch1, "S11", port1, window2)
```

or

```
Pna.Channels.Add(2)
```

The latter will have no visible effect on the analyzer. It will simply create channel 2 if it does not already exist.

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

 [Loading and Writing Calibration data.](#)

(**Bold** Methods or Properties provide access to a child object)

Methods	Interface	Description
Abort	IChannel	Aborts the current measurement sweep on the channel.
AveragingRestart	IChannel	Clears and restarts averaging of the measurement data.
Continuous	IChannel	The channel continuously responds to trigger signals.
CopyToChannel	IChannel	Sets up another channel as a copy of this object's channel.
GetNumberOfGroups	IChannel3	Returns the <u>number of groups</u> a channel has yet to acquire.

<u>getSourcePowerCalData</u>	IChannel	OBSOLETE - use <u>Get SourcePowerCalDataEx Method</u>
<u>getSourcePowerCalDataEx</u>	IChannel4	Returns requested source power calibration data, if it exists.
<u>GetXAxisValues</u>	IChannel	Returns the channel's X-axis values into a dimensioned Variant array.
<u>GetXAxisValues2</u>	IChannel	Returns the channel's X-axis values into a dimensioned NON-Variant array.
<u>Hold</u>	IChannel	Puts the Channel in Hold - not sweeping.
<u>Next_IFBandwidth</u>	IChannel	A function that returns the Next higher IF Bandwidth value.
<u>NumberOfGroups</u>	IChannel	Sets the Number of trigger signals the channel will receive.
<u>Preset</u>	IChannel	Resets the channel to factory defined settings.
<u>PreviousIFBandwidth</u>	IChannel	Returns the previous IF Bandwidth value.
<u>putSourcePowerCalData</u>	IChannel	OBSOLETE - use <u>Put SourcePowerCalDataEx Method</u>
<u>putSourcePowerCalDataEx</u>	IChannel4	Inputs source power calibration data to this channel for a specific source port.
<u>SelectCal Set</u>	IChannel	Specifies the Cal Set to use for the Channel
<u>Single</u>	IChannel	Channel responds to one trigger signal from any source (internal, external, or manual). Then channel switches to Hold.

Properties	Interface	Description
<u>AlternateSweep</u>	IChannel	Sets sweeps to either alternate or chopped.
<u>Attenuator</u>	IChannel	Sets or returns the value of the attenuator control for the specified port number.
<u>AttenuatorMode</u>	IChannel	Sets or returns the mode of operation of the attenuator control for the specified port number.
<u>Averaging</u>	IChannel	Turns trace averaging ON or OFF for all measurements on the channel.
<u>AveragingCount</u>	IChannel	Returns the number of sweeps that have been averaged into the measurements.
<u>AveragingFactor</u>	IChannel	Specifies the number of measurement sweeps to combine for an average.
<u>BalancedTopology</u>	IChannel6	Sets and returns the topology of a balanced DUT.
<u>Calibrator</u>	IChannel4	Used to perform an Unguided calibration.
<u>CalSet</u>	IChannel	

<u>centerFrequency</u>	IChannel	Sets or returns the center frequency of the channel. Shared with the Segment Object
<u>channelNumber</u>	IChannel	Returns the Channel number. Shared with the Measurement Object
<u>CoupleChannelParams</u>	IChannel5	Turns ON and OFF Time Domain Trace Coupling.
<u>CouplePorts</u>	IChannel	Turns ON and OFF port power coupling.
<u>CWFrequency</u>	IChannel	Set the Continuous Wave (CW) frequency.
<u>DwellTime</u>	IChannel	Sets or returns the dwell time for the channel. Shared with the Segment Object
<u>ErrorCorrection</u>	IChannel7	Attempts to sets error correction ON or OFF for all of the measurements on the channel.
<u>ExternalTriggerDelay</u>	IChannel6	Sets or returns the external trigger delay value for the channel.
Fixturing	IChannel6	Port Ext, Embedding, and De-embedding functions.
<u>FrequencyOffsetDivisor</u>	IChannel2	Part of formula used to determine offset frequency of receivers.
<u>FrequencyOffsetFrequency</u>	IChannel2	Part of formula used to determine offset frequency of receivers.
<u>FrequencyOffsetMultiplier</u>	IChannel2	Part of formula used to determine offset frequency of receivers.
<u>FrequencyOffsetCWOverride</u>	IChannel2	Establishes a fixed (CW) stimulus frequency while measuring swept response frequency range.
<u>FrequencyOffsetState</u>	IChannel2	Turns frequency Offset ON and OFF.
<u>FrequencySpan</u>	IChannel	Sets or returns the frequency span of the channel. Shared with the Segment Object.
<u>IFBandwidth</u>	IChannel	Sets or returns the IF Bandwidth of the channel. Shared with the Segment Object.
IFConfiguration	IChannel4	Control the IF gain and source path settings for the H11 Option.
<u>IsContinuous</u>	IChannel3	Returns whether or not a channel is in <u>continuous</u> mode.
<u>IsHold</u>	IChannel3	Returns whether or not a channel is in <u>hold</u> mode.
<u>NumberOfPoints</u>	IChannel	Sets or returns the Number of Points of the channel. Shared with the Segment Object.
<u>Parent</u>	IChannel	Returns a handle to the parent object of the channel.
<u>PowerSlope</u>	IChannel	Sets or returns the Power Slope value.
<u>R1InputPath</u>	IChannel2	Throws internal reference switch (<u>option 081</u>).

<u>ReceiverAttenuator</u>	IChannel	Sets or returns the value of the specified receiver attenuator control.
<u>ReduceIFBandwidth</u>	IChannel	Sets or returns the state of the <u>Reduced IF Bandwidth at Low Frequencies</u> setting.
<u>Segments</u>	IChannel	Collection for iterating through the sweep segments of a channel.
<u>SourcePowerCalPowerOffset</u>	IChannel4	Sets or returns a power level offset from the PNA test port power.
<u>SourcePowerCorrection</u>	IChannel	Turns source power correction ON or OFF for a specific source port.
<u>StartFrequency</u>	IChannel	Sets or returns the start frequency of the channel. Shared with the Segment Object
<u>StartPower</u>	IChannel	Sets the start power of the analyzer when sweep type is set to Power Sweep.
<u>StopFrequency</u>	IChannel	Sets or returns the stop frequency of the channel. Shared with the Segment Object
<u>StopPower</u>	IChannel	Sets the Stop Power of the analyzer when sweep type is set to Power Sweep.
<u>SweepGenerationMode</u>	IChannel	Sets the method used to generate a sweep: continuous ramp (analog) or discrete steps (stepped).
<u>SweepTime</u>	IChannel	Sets the Sweep time of the analyzer.
<u>SweepType</u>	IChannel	Sets the type of X-axis sweep that is performed on a channel.
<u>TestPortPower</u>	IChannel	Sets or returns the RF power level for the channel. Shared with the Segment Object
<u>TriggerMode</u>	IChannel	Determines the measurement that occurs when a trigger signal is sent to the channel.
<u>UserRangeMax</u>	IChannel	Sets the stimulus stop value for the specified User Range.
<u>UserRangeMin</u>	IChannel	Sets the stimulus start value for the specified User Range.
<u>XAxisPointSpacing</u>	IChannel	Sets X-Axis point spacing for the active channel.

IChannel History

Interface	Introduced with PNA Rev:
IChannel	1.0
IChannel2	3.0
IChannel3	4.0
IChannel4	4.0
IChannel5	4.2
IChannel6	5.0
IChannel7	5.2

ISourcePowerCalData Interface

Description

Contains methods for putting source power calibration data in and getting source power calibration data out of the analyzer using typed data. The methods in this interface transfer data more efficiently than methods that use variant data.

Note: Interface **ISourcePowerCalData** is abbreviated as **ISPCD** in the following table.

Methods	Interface	Description
	<u>See History</u>	
<u>getSourcePowerCalDataScalar</u>	ISPCD	OBSOLETE - use <u>PutSourcePowerCalDataScalarEx Method</u>
<u>getSourcePowerCalDataScalarEx</u>	ISPCD2	Returns requested source power calibration data, if it exists.
<u>putSourcePowerCalDataScalar</u>	ISPCD	OBSOLETE - use <u>PutSourcePowerCalDataEx Method</u>
<u>putSourcePowerCalDataScalarEx</u>	ISPCD2	Inputs source power calibration data to a channel, for a specific source port.
Properties	Description	
None		

ISourcePowerCalData History

Interface	Introduced with PNA Rev:
ISourcePowerCalData	2.0
ISourcePowerCalData2	4.0

Channels Collection

Description

A collection object that provides a mechanism for iterating through the channels

Collections are, by definition, unordered lists of like objects. You cannot assume that Channels.Item(1) is always Channel 1.

Accessing the Channels collection

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)
```

```
Dim chans As Channels
Set chans = app.Channels
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Interface	Description
Add	IChannels	An alternate way to create a measurement.
Hold	IChannels	Places all channels in Hold trigger mode.
Item	IChannels2	Use to get a handle on a channel in the collection.
Resume	IChannels2	Resumes the trigger mode of all channels that was in effect before sending the channels.Hold method.

Properties		Description
Count	IChannels	Returns the number of channels in the analyzer.
Parent	IChannels	Returns a handle to the current Application.
UnusedChannelNumbers	IChannels2	Returns an array of channel numbers that are NOT in use.
UsedChannelNumbers	IChannels2	Returns an array of channel numbers that are in use.

Fixturing Object

Description

Contains the properties for Embedding and De-embedding test fixtures.

Accessing the Fixturing object

```
Dim app as AgilentPNA835x.Application
Dim chan as Channel
Set chan = app.ActiveChannel
Dim fixt as Fixturing
Set fixt = chan.Fixturing
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[About Fixturing](#)

Methods		Description
AutoPortExtMeasure	IFixturing2	Measures either an OPEN or SHORT standard.
AutoPortExtReset	IFixturing2	Clears old port extension delay and loss data.

Properties	Interface	Description
	See History	
AutoPortExtConfig	IFixturing2	Sets the frequency span that is used to calculate Automatic Port Extension.
AutoPortExtDCOffset	IFixturing2	Specifies whether or not to include DC Offset as part of Automatic port extension.
AutoPortExtLoss	IFixturing2	Specifies whether or not to include loss correction as part of Automatic Port Extension.
AutoPortExtSearchStart	IFixturing2	Set the start frequency for custom user span.
AutoPortExtSearchStop	IFixturing2	Set the stop frequency for custom user span.
AutoPortExtState	IFixturing2	Enables and disables automatic port extensions on the specified port.
CmnModeZConvPortImag	IFixturing2	Sets imaginary value for common port impedance conversion.
CmnModeZConvPortReal	IFixturing2	Sets real value for common port impedance conversion.

<u>CmnModeZConvState</u>	IFixturing2	Turns ON/OFF common port impedance conversion.
<u>CmnModeZConvPortZ0</u>	IFixturing2	Sets impedance value for common port impedance conversion.
<u>DiffPortMatch_C</u>	IFixturing2	Sets Capacitance value of the differential matching circuit.
<u>DiffPortMatch_G</u>	IFixturing2	Sets Conductance value of the differential matching circuit.
<u>DiffPortMatch_L</u>	IFixturing2	Sets Inductance value of the differential matching circuit.
<u>DiffPortMatch_R</u>	IFixturing2	Sets Resistance value of the differential matching circuit.
<u>DiffPortMatchMode</u>	IFixturing2	Sets type of circuit to embed.
<u>DiffPortMatchUserFilename</u>	IFixturing2	Specifies the 4-port touchstone file for user-defined differential matching circuit.
<u>DiffPortMatchState</u>	IFixturing2	Turns ON/OFF differential matching circuit function.
<u>DiffZConvPortImag</u>	IFixturing2	Sets imaginary value for differential port impedance conversion.
<u>DiffZConvPortReal</u>	IFixturing2	Sets real value for differential port impedance conversion.
<u>DiffZConvPortZ0</u>	IFixturing2	Sets impedance value for differential port impedance conversion.
<u>DiffZConvState</u>	IFixturing2	Turns ON/OFF differential port impedance conversion.
<u>Embed4PortA</u>	IFixturing2	Returns PNA portA connections.
<u>Embed4PortB</u>	IFixturing2	Returns PNA portB connections.
<u>Embed4PortC</u>	IFixturing2	Returns PNA portC connections.
<u>Embed4PortD</u>	IFixturing2	Returns PNA portD connections.
<u>Embed4PortList</u>	IFixturing2	Specifies all PNA port connections.
<u>Embed4PortNetworkFilename</u>	IFixturing2	Specifies *.s4p filename.
<u>Embed4PortNetworkMode</u>	IFixturing2	Specify embed, de-embed, or none.
<u>Embed4PortState</u>	IFixturing2	Turns ON or OFF 4-port Network Embed/De-embed.
<u>Embed4PortTopology</u>	IFixturing2	Specifies the PNA / DUT topology.

<u>FixturingState</u>	IFixturing	Turns Fixturing ON and OFF on this channel.
<u>Port2PdeembedCktModel</u>	IFixturing	Sets and returns the 2 port De-embedding circuit model for the specified port number.
<u>Port2PdeembedState</u>	IFixturing	Turns 2 port de-embedding ON and OFF on this channel.
<u>PortArbzImag</u>	IFixturing3	Sets and returns the imaginary impedance value for the specified single-ended port number.
<u>PortArbzReal</u>	IFixturing3	Sets and returns the real impedance value for the specified single-ended port number.
<u>PortArbzState</u>	IFixturing	Turns single-ended port impedance ON and OFF on the specified channel.
<u>PortArbzZ0</u>	IFixturing3	Sets and returns the real and imaginary impedance value for the specified single-ended port number.
<u>PortDelay</u>	IFixturing	Sets and returns the Port Delay value for the specified port number.
<u>PortExtState</u>	IFixturing	Turns Port Extension ON and OFF on this channel.
<u>PortExtUse1</u>	IFixturing	Sets and returns the USE1 ON/OFF state for the Loss1 and Freq1 values for the specified port number.
<u>PortExtUse2</u>	IFixturing	Sets and returns the USE2 ON/OFF state for the Loss2 and Freq2 values for the specified port number.
<u>PortFreq1</u>	IFixturing	Sets and returns the 1st Port Frequency value for the specified port number.
<u>PortFreq2</u>	IFixturing	Sets and returns the 2nd Port Frequency value for the specified port number.
<u>PortLoss1</u>	IFixturing	Sets and returns the 1st Port Loss value for the specified port number.
<u>PortLoss2</u>	IFixturing	Sets and returns the 2nd Port Loss value for the specified port number.
<u>PortLossDC</u>	IFixturing	Sets and returns the Port Loss at DC value for the specified port number.
<u>PortMatching_C</u>	IFixturing	Sets and returns the Capacitance, 'C' value for the specified port number.

<u>PortMatching_G</u>	IFixturing	Sets and returns the Conductance, 'G' value for the specified port number.
<u>PortMatching_L</u>	IFixturing	Sets and returns the Inductance, 'L' value for the specified port number.
<u>PortMatching_R</u>	IFixturing	Sets and returns the Resistance, 'R' value for the specified port number.
<u>PortMatchingCktModel</u>	IFixturing	Sets and returns the Port Matching circuit model for the specified port number.
<u>PortMatchingState</u>	IFixturing	Turns Port Matching ON and OFF on this channel.
<u>strPort2Pdeembed_S2PFile</u>	IFixturing	Sets and returns the 2 port De-embedding 'S2P' file name for the specified port number.
<u>strPortMatch_S2PFile</u>	IFixturing	Sets and returns the Port Matching 'S2P' file name for the specified port number.

IFixturing History

Interface	Introduced with PNA Rev:
IFixturing	5.0
IFixturing2	5.2
IFixturing3	5.25

Gating Object

Description

Contains the methods and properties that control Time Domain Gating.

Accessing the Gating Object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim gate As Gating
Set gate = app.ActiveMeasurement.Gating
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Time Domain Topics](#)

Methods

None

Properties

Interface

Description

[\(see History\)](#)

[Center](#)

IGating

Sets or returns the Center time.
Shared with the Transform Object

[CoupledParameters](#)

IGating2

Select Gating parameters to couple

[Shape](#)

IGating

Specifies the shape of the gate filter.

 [Span](#)

IGating

Sets or returns the Span time.
Shared with the Transform Object

[Start](#)

IGating

Sets or returns the Start time.
Shared with the Transform Object

[State](#)

IGating

Turns an Object ON and OFF.

[Stop](#)

IGating

Sets or returns the Stop time.
Shared with the Transform Object

[Type](#)

IGating

Specifies the type of gate filter used.

History

Interface	Introduced with PNA Rev:
------------------	---------------------------------

IGating	1.0
---------	-----

IGating2	4.2
----------	-----

GuidedCalibration Object

Description

Contains the methods and properties used to perform a Guided Calibration.


Accessing the GuidedCalibration object

```
Dim app as AgilentPNA835x.Application
Dim CalMgr
Set CalMgr = App.GetCalManager
Dim guidedCal
Set guidedCal = CalMgr.GuidedCalibration
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods		Description
AcquireStep	IGuidedCalibration	Acquire data for a cal step.
ApplyDeltaMatchFromCalSet Method	IGuidedCalibration2	Apply a cal as Delta Match Cal.
GenerateErrorTerms	IGuidedCalibration	Generates the error terms for the calibration.
GenerateGlobalDeltaMatchSequence	IGuidedCalibration2	Initiates a global delta match calibration.
GenerateSteps	IGuidedCalibration	Request to generate a connection list and return the number of steps required.
 GetStepDescription	IGuidedCalibration	Query description of a step.
Initialize	IGuidedCalibration	Initial setup with channel context for the remote cal object.

Properties	Interface	Description
	See History	
CalKitType	IGuidedCalibration	Sets the cal kit for the port.
CompatibleCalKits	IGuidedCalibration	Returns the list of cal kits for the port.
ConnectorType	IGuidedCalibration	Sets the connector type for the port.

<u>PortsNeedingDeltaMatch</u>	IGuidedCalibration2	Returns port numbers that need delta match cal.
<u>ThruCalMethod</u>	IGuidedCalibration	Sets the THRU method for the calibration.
<u>ThruPortList</u>	IGuidedCalibration	Sets the thru connection port pairs.
<u>ValidConnectorTypes</u>	IGuidedCalibration	Get Valid Connector Types.

IGuidedCalibration History

Interface	Introduced with PNA Rev:
IGuidedCalibration	5.0
IGuidedCalibration2	5.25

HWAuxIO Object

Description

Contains the methods and properties that control the rear panel Auxiliary Input / Output connector.

Accessing the HWAuxIO object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)


Dim AuxIO As HWAuxIO
Set AuxIO = app.GetAuxIO
```

See Also:

[Pinout of the Aux IO Connector](#)

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods	Interface	Description
get_InputVoltage	IHWAuxIO	Reads the ADC input voltage
get_OutputVoltage	IHWAuxIO	Reads voltages on the DAC/Analog Output 1 and Output 2
get_OutputVoltageMode	IHWAuxIO2	Reads mode setting for either DAC output.
get_PortCData	IHWAuxIO	Reads a 4-bit value from Port C
put_OutputVoltage	IHWAuxIO	Writes voltages to the DAC/Analog Output 1 and Output 2
 put_OutputVoltageMode	IHWAuxIO2	Writes mode setting for either DAC output.
put_PortCData	IHWAuxIO	Writes a 4-bit value to Port C

Properties		Description
FootSwitch	IHWAuxIO	Reads the Footswitch Input
FootswitchMode	IHWAuxIO3	Determines the action that occurs when the footswitch is pressed.
PassFailLogic	IHWAuxIO	Sets and reads the logic of the PassFail line Shared with the HWMaterialHandler Object

<u>PassFailMode</u>	IHWAuxIO	Sets and reads the mode of the PassFail line Shared with the HWMaterialHandler Object
<u>PassFailPolicy</u>	IHWAuxIO4	Sets the policy used to determine how global pass/fail is computed. Shared with the HWMaterialHandler Object
<u>PassFailScope</u>	IHWAuxIO	Sets and reads the scope of the PassFail line Shared with the HWMaterialHandler Object
<u>PassFailStatus</u>	IHWAuxIO4	Returns the most recent pass/fail status value. Shared with the HWMaterialHandler Object
<u>PortCLogic</u>	HWAuxIO	Sets and reads the logic mode of Port C
<u>PortCMode</u>	HWAuxIO	Sets and reads the mode of Port C
<u>SweepEndMode</u>	HWAuxIO	Sets and reads the event that causes the Sweep End line to go to a false state. Shared with the HWMaterialHandler Object

IHWAuxIO History

Interface	Introduced with PNA Rev:
IHWAuxIO	2.0
IHWAuxIO2	3.0
IHWAuxIO3	3.0
IHWAuxIO4	5.0

HWExternalTestSetIO Object

Description

Contains the methods and properties that control the rear panel External Test Set Input / Output connector

Accessing the HWExternalTestSetIO object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim ExtTS As HWExternalTestSetIO
Set ExtTS = app.GetExternalTestSetIO
```

See Also:


[Pinout of the Aux IO Connector](#)

[Pinout for the External Test Set Connector](#)

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods	Description
ReadData	Reads data and generates the appropriate timing signals
ReadRaw	Reads data, but does NOT generate appropriate timing signals
WriteData	Writes data and generates the appropriate timing signals
WriteRaw	Writes data, but does NOT generate the appropriate timing signals

Properties	Description
 Interrupt	Returns the state of the Interrupt line
SweepHoldOff	Returns the state of the Sweep Holdoff line

IHWExternalTestSetIO History

Interface	Introduced with PNA Rev:
HWExternalTestSetIO	2.0

HWMaterialHandlerIO Object

Description

Contains the methods and properties that control the rear panel Material Handler Input / Output connector.

Accessing the HWMaterialHandlerIO object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)


Dim MatHdlr As HWMaterialHandlerIO
Set MatHdlr = app.GetMaterialHandlerIO
```

See Also:

[Pinout for the Material HandlerIO Connector](#)

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods	Interface	Description
get_Input1	HWMaterialHandlerIO	Reads a hardware latch that captures low to high transition on Input1
get_Output	HWMaterialHandlerIO	Returns the last value written to the selected output pin.
get_Port	HWMaterialHandlerIO	Returns the value from the specified "readable" port.
put_Output	HWMaterialHandlerIO	Writes a TTL HI or TTL Low to output pins 3 or 4.
 t_Port	HWMaterialHandlerIO	Writes a value to the specified port.

Properties		Description
IndexState	HWMaterialHandlerIO2	Determines the control of Material Handler connector Pin 20
ReadyForTriggerState	HWMaterialHandlerIO2	Determines the control of Material Handler connector Pin 21
PassFailLogic	HWMaterialHandlerIO	Sets and reads the logic of the PassFail line Shared with the HWAuxIO Object

<u>PassFailMode</u>	HWMaterialHandlerIO	Sets and reads the mode for the PassFail line Shared with the HWAuxIO Object
<u>PassFailPolicy</u>	HWMaterialHandlerIO2	Sets the policy used to determine how global pass/fail is computed. Shared with the HWAuxIO Object
<u>PassFailScope</u>	HWMaterialHandlerIO	Sets and reads the scope for the PassFail line Shared with the HWAuxIO Object
<u>PassFailStatus</u>	HWMaterialHandlerIO2	Returns the most recent pass/fail status value. Shared with the HWAuxIO Object
<u>PortLogic</u>	HWMaterialHandlerIO	Sets and returns the logic mode of data ports A-H
<u>PortMode</u>	HWMaterialHandlerIO	Sets and returns whether Port C or Port D is used for writing or reading data
<u>SweepEndMode</u>	HWMaterialHandlerIO	Sets and reads the event that cause the Sweep End line to go to a low state. Shared with the HWAuxIO Object

HWMaterialHandlerIO History

Interface	Introduced with PNA Rev:
HWMaterialHandlerIO	2.0
HWMaterialHandlerIO2	5.0

IFConfiguration Object

Description

These properties control the IF gain and source path settings for the H11 Option.

Accessing the IFConfiguration object

```
Dim app as AgilentPNA835x.Application
Dim chan as Channel
Set chan = app.ActiveChannel
Dim cfg as IIFConfiguration
Set cfg = chan.IFConfiguration
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[About the H11 Option](#)

[Pulsed Application](#)

[ConfigNarrowBand2 Method](#)


[Pulsed Measurement Example](#)

Methods	Description
---------	-------------

None

Properties	Interface	Description
------------	-----------	-------------

[See History](#)

 IFFilterSampleCount	IFConfiguration2	Sets or returns the number of taps in the IF filter.
IFFilterSamplePeriod	IFConfiguration2	Sets or returns the IF filter sample period time.
IFFilterSamplePeriodList	IFConfiguration2	Returns the list of available IF filter sample periods for the instrument.
IFFilterSamplePeriodMode	IFConfiguration2	Sets or returns the IF filter sample period mode.(Auto or Manual).
IFFilterSource Property	IFConfiguration2	Sets or retrieves type of IF filter to be used.
IFGainLevel Property	IFConfiguration	Sets the gain level for the specified receiver.
IFGainMode Property	IFConfiguration	Sets the gain state for ALL receivers.

<u>IFGateEnable Property</u>	IFConfiguration2	Sets or retrieves the state of the IF Gate.
<u>IFSourcePath Property</u>	IFConfiguration	Sets the source path of the specified receiver to Internal or External.
<u>MaximumIFFilterSampleCount</u>	IFConfiguration2	Returns the maximum allowed value for the IFFilterSampleCount.
<u>MinimumIFFilterSampleCount</u>	IFConfiguration2	Returns the minimum allowed value for the IFFilterSampleCount.

IFConfiguration History

Interface	Introduced with PNA Rev:
IIFConfiguration	4.0
IIFConfiguration2	4.0

IMixer Interface (Option 083)

Description

Contains the methods and properties to setup Mixer measurements. For performing calibrations, use either the [SMC Type Object](#) or the [VMC Type Object](#).

Accessing the IMixer Interface

Access the IMixer Interface through the Measurement Object. If the particular type of Measurement that was created supports IMixer, then the program determines this at run time and can access the functionality exposed by IMixer. Because the determination of IMixer support is not made until runtime, the program should handle the case where IMixer is not supported on the object.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", "analyzerName")
app.Preset

' FCA Measurements can't share the channel with standard measurements
' Because preset creates a single measurement in channel 1, we first delete the
standard measurement
Dim standardMeas As IMeasurement
Set standardMeas = app.ActiveMeasurement
standardMeas.Delete

' Create a Measurement object, in this case using the IMeasurement interface
Dim meas As IMeasurement
Set meas = app.CreateCustomMeasurementEx(1, "SMC_Forward.SMC_ForwardMeas", "SC21")

' See if this measurement object supports IMixer
Dim mixer As IMixer
```

See an example program that shows how to create and calibrate a standard [SMC](#) or [VMC](#) measurement or a [fixed output SMC](#) measurement.

See Also:

[PNA Automation Interfaces](#)

[PNA Object Model](#)



Methods	Interface	Description
	See History	
Apply	IMixer3	Applies mixer settings.
Calculate	IMixer	Automatically calculate Input and Output frequencies for mixer setup.
LoadFile	IMixer	Loads a previously-configured mixer attributes file (.mxr)
SaveFile	IMixer	Saves the settings for the mixer/converter test setup to a mixer attributes file.

Properties		Description
<u>ActiveXAxisRange</u>	IMixer3	Sets or returns the swept parameter to display on the X-axis.
<u>AvoidSpurs</u>	IMixer	Sets and returns the state of the avoid spurs feature.
<u>IFDenominator</u>	IMixer	Sets or returns the denominator value of the IF Fractional Multiplier.
<u>IFNumerator</u>	IMixer	Sets or returns the numerator value of the IF Fractional Multiplier.
<u>IFSideband</u>	IMixer	Sets or returns the value of the IF sideband.
<u>IFStartFrequency</u>	IMixer	Returns the start frequency of the mixer IF.
<u>IFStopFrequency</u>	IMixer	Returns the stop frequency of the mixer IF.
<u>InputDenominator</u>	IMixer	Sets or returns the denominator value of the Input Fractional Multiplier.
<u>InputNumerator</u>	IMixer	Sets or returns the numerator value of the Input Fractional Multiplier.
<u>InputPower</u>	IMixer	Sets or returns the value of the Input Power.
<u>InputStartFrequency</u>	IMixer	Sets or returns the start frequency of the mixer input.
<u>InputStopFrequency</u>	IMixer	Sets or returns the stop frequency of the mixer input.
<u>IsInputGreaterThanLO</u>	IMixer2	Specifies whether to use the Input frequency that is greater than the LO or less than the LO.
<u>LODenominator</u>	IMixer	Sets or returns the denominator value of the LO Fractional Multiplier.
<u>LOFixedFrequency</u>	IMixer	Sets or returns the fixed frequency of the specified LO.
<u>LOName</u>	IMixer	Sets or returns the LO name.
<u>LONumerator</u>	IMixer	Sets or returns the numerator value of the LO Fractional Multiplier.
<u>LOPower</u>	IMixer	Sets or returns the value of the LO Power.
<u>LORangeMode</u>	IMixer3	Sets or returns the LO sweep mode to fixed or swept.
<u>LOStage</u>	IMixer	Returns the number of stages.
<u>LOStartFrequency</u>	IMixer3	Sets or returns the start frequency of the specified LO.
<u>LOStopFrequency</u>	IMixer3	Sets or returns the start frequency of the specified LO.
<u>OutputFixedFrequency</u>	IMixer3	Sets or returns the fixed frequency of the mixer output.
<u>OutputSideband</u>	IMixer	Sets or returns the value of the output sideband.
<u>OutputStartFrequency</u>	IMixer	Sets or returns the start frequency of the mixer output.
<u>OutputStopFrequency</u>	IMixer	Sets or returns the stop frequency of the mixer output.

IMixer History

Interface	Introduced with PNA Rev:
IIMixer	1.0
IIMixer2	3.5
IIMixer3	4.0

InterfaceControl Object

Description

Contains the methods and properties that support Interface Control.

Accessing the InterfaceControl object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim IntControl As InterfaceControl
Set IntControl = app.InterfaceControl
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Interface Control Feature](#)

Methods	Interface	Description
---------	-----------	-------------

ConfigurationFile	InterfaceControl	Recalls an Interface Control file
-----------------------------------	------------------	-----------------------------------

Properties	Description
------------	-------------

State	InterfaceControl	Turns Interface Control ON and OFF
-----------------------	------------------	------------------------------------

InterfaceControl History

Interface	Introduced with PNA Rev:
-----------	--------------------------

InterfaceControl	5.2
------------------	-----

Limit Test Collection

Description

Child of the **Measurement** Object. A collection that provides a mechanism for iterating through the Measurement's Limit Segment objects (Limit Lines). The collection has 100 limit lines by default.

Accessing the LimitTest collection

Get a handle to an individual limit segment by specifying an item of the [LimitTest](#) collection.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim limSegs As LimitTest
Set limSegs = app.ActiveMeasurement.LimitTest
limSegs.Item(1).BeginResponse = 1000000000#
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

[Limit Line Testing Example](#)

Methods	Description
GetTestResult	Retrieves the Pass/Fail results of the Limit Test (State).
Item	Use to get a handle on a limit line in the collection.

Properties	Description
Count	Returns the number of limit lines used in the measurement.
LineDisplay	Displays the limit lines on the screen.
SoundOnFail	Enables a beep on Limit Test fails.
State	Turns ON and OFF limit testing.

LimitTest History

Interface	Introduced with PNA Rev:
ILimitTest	1.0

LimitSegment Object

Description

The LimitSegment object is an individual limit line.

Accessing the LimitSegment object

Get a handle to an individual limit line by using the LimitTest collection.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim limSegs As LimitTest
Set limSegs = app.ActiveMeasurement.LimitTest
limSegs(1).BeginResponse = 10000000000#
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods	Description
---------	-------------

None

Properties	Description
------------	-------------

[BeginResponse](#) Specifies the Y-axis value that corresponds with Begin Stimulus (X-axis) value.

[BeginStimulus](#) Specifies the beginning X-axis value of the Limit Line.

[EndResponse](#) Specifies the Y-axis value that corresponds with End Stimulus (X-axis) value.

[EndStimulus](#) Specifies the End X-axis value of the Limit Line.



[Type](#)

Specifies the Limit Line type.

LimitSegment History

Interface	Introduced with PNA Rev:
ILimitSegment	1.0

Marker Object

Description

Contains the methods and properties that control Markers. There are 10 markers available per measurement:

- 1 reference marker
- 9 markers for absolute data or data relative to the reference marker (delta markers).

There are two ways to control markers through COM.

1. The Measurement object has properties that apply to ALL of the markers for that measurement. For example, **meas.MarkerFormat = naLinMag** applies formatting to all markers.
2. Marker object properties override the Measurement object properties. For example, you can then override the format setting for an individual marker by specifying **mark.Format = naLogMag** on the marker object.

Note: SearchFilterBandwidth is available through the measurement object.

Accessing the Marker object

To turn ON a marker, get a handle to the marker through the measurement object. If not already activated, this command will turn ON marker 1

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

app.ActiveMeasurement.marker(1).Format = naLinMag
```

You can also set the marker object to an object variable:

```
Dim m1 As Marker
Set m1 = app.ActiveMeasurement.Marker(1)
m1.Format = naMarkerFormat_LinMag
```

See Also:

[PNA Automation Interfaces](#)

[PNA Object Model](#)

Methods	Interface	Description
Activate	IMarker	Makes an object the Active Object. Shared with the Marker Object
SearchMax	IMarker	Searches the marker domain for the maximum value.
SearchMin	IMarker	Searches the marker domain for the minimum value.
SearchNextPeak	IMarker	Searches the marker's domain for the next largest peak value.

<u>SearchPeakLeft</u>	IMarker	Searches the marker's domain for the next VALID peak to the left of the marker.
<u>SearchPeakRight</u>	IMarker	Searches the marker's domain for the next VALID peak to the right of the marker.
<u>SearchTarget</u>	IMarker	Searches the marker's domain for the target value.
<u>SearchTargetLeft</u>	IMarker	Moving to the left of the marker position, searches the marker's domain for the target value.
<u>SearchTargetRight</u>	IMarker	Moving to the right of the marker position, searches the marker's domain for the target value.
<u>SetCenter</u>	IMarker	Changes the analyzer's center frequency to the X-axis position of the marker.
<u>SetCW</u>	IMarker	Changes the analyzer to sweep type CW mode and makes the CW frequency the marker's frequency.
<u>SetElectricalDelay</u>	IMarker	Changes the measurement's electrical delay to the marker's delay value.
<u>SetReferenceLevel</u>	IMarker	Changes the measurement's reference level to the marker's Y-axis value.
<u>SetStart</u>	IMarker	Changes the analyzer's start frequency to the X-axis position of the marker.
<u>SetStop</u>	IMarker	Changes the analyzer's stop frequency to the X-axis position of the marker.

Properties		Description
<u>Bucket Number</u>	IMarker	Marker data point number
<u>DeltaMarker</u>	IMarker	Makes a marker relative to the reference marker
<u>Distance</u>	IMarker2	Sets or returns distance value for time domain trace.
<u>Format</u>	IMarker	Linear, SWR, and so forth
<u>Interpolated</u>	IMarker	Turn marker interpolation ON and OFF
<u>Number</u>	IMarker	Read the number of the active marker
<u>PeakExcursion</u>	IMarker	Sets and reads the peak excursion value for the specified marker.
<u>PeakThreshold</u>	IMarker	Sets peak threshold for the specified marker.
<u>SearchFunction</u>	IMarker	Emulates the Tracking function in the marker search dialog box.
<u>Stimulus</u>	IMarker	Sets and reads the X-Axis value of the marker.
<u>Target Value</u>	IMarker	Sets the target value for the marker when doing Target Searches.

<u>Tracking</u>	IMarker	The tracking function finds the selected search function every sweep.
<u>Type</u>	IMarker	Sets and reads the marker type.
<u>UserRange</u>	IMarker	Assigns the marker to the specified User Range.
<u>UserRangeMax</u>	IMarker	Sets the stimulus stop value for the specified User Range.
<u>UserRangeMin</u>	IMarker	Sets the stimulus start value for the specified User Range.
<u>Value</u>	IMarker	Reads the Y-Axis value of the marker.

Marker History

Interface	Introduced with PNA Rev:
IMarker	1.0
IMarker2	4.2

Measurement Object

See [IArrayTransfer Interface](#) for putting and getting typed data.

See [IMixer Interface](#) (used with [Option 083](#))

Description

The Measurement object is probably the most used object in the PNA Object Model. A measurement object represents the chain of data processing algorithms that take raw data from the channel and make it ready for display, which then becomes the scope of the [Trace object](#).

A Measurement object is defined by its parameter (S11, S22, A/R1, B and so forth). The measurement object is associated with a [channel](#) which drives the hardware that produces the data that feeds the measurement. The root of a measurement is the raw data. This buffer of complex paired data then flows through a number of processing blocks: error-correction, trace math, phase correction, time domain, gating, formatting. All of these are controlled through the measurement object.

The ACTIVE measurement is the measurement that will be acted upon if you make a setting from the front panel. It is the measurement whose "button" is pressed in the window with the red "active window" frame. If you create a new measurement, that measurement becomes the active measurement.

Therefore, all automation methods with the word "Active" in them refer to the object associated with the Active measurement, whether that object is a Channel, Window, Trace or Limit line.

Learn about the [IMeasurement2 Interface](#) for reading stimulus properties.

Accessing the Measurement object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim meas As IMeasurement
Set meas = app.ActiveMeasurement
```

or

```
Set meas = app.Measurements(n)
```

You can access four other objects through the Measurement object: markers, limit test, transform, and gating. For example, because each measurement has its own set of markers, you can set a marker by doing this:

```
Dim meas as measurement
Set meas = app.ActiveMeasurement
meas.marker(1).Stimulus = 900e6
```

IMeasurement2 Interface

Some of the properties and methods for the IMeasurement2 Interface return stimulus values that are set using the channel object. The following is the reason these properties and methods are duplicated.

Every measurement carries with it a snapshot of the stimulus properties of the channel that were in effect when the measurement last acquired data. Therefore, it is the measurement that provides the most accurate stimulus description of its data. Any change made to the channel after the measurement was acquired renders the IChannel interface unreliable in terms of describing the measurement.

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

(**Bold** Methods or Properties provide access to a child object)

Methods	Interface	Description
<u>Activate</u>	IMeasurement	Makes an object the Active Object. Shared with the Marker Object
<u>ActivateMarker</u>	IMeasurement	Makes a marker the Active Marker.
<u>ChangeParameter</u>	IMeasurement	Changes the parameter of the measurement.
<u>DataToDivisor</u>	IMeasurement	Stores data for receiver power cal of unratioed measurements.
<u>DataToMemory</u>	IMeasurement	Stores the active measurement into memory.
<u>Delete</u>	IMeasurement	Deletes the measurement object.
<u>DeleteAllMarkers</u>	IMeasurement	Deletes all of the markers from the measurement.
<u>DeleteMarker</u>	IMeasurement	Deletes a marker from the active measurement.
<u>getData</u>	IMeasurement	Retrieves Complex data from analyzer memory
<u>getDataByString</u>	IMeasurement	Retrieves variant data from the specified location in your choice of formats.
<u>GetFilterStatistics</u>	IMeasurement	Returns all four Filter Statistics
<u>GetReferenceMarker</u>	IMeasurement	Returns a handle to the reference marker.
<u>Get SnPData</u>	IMeasurement3	Returns SnP data.
<u>GetTraceStatistics</u>	IMeasurement	Returns the Trace Statistics.
<u>GetXAxisValues</u>	IMeasurement2	Returns the stimulus values for the measurement.
<u>InterpolateMarkers</u>	IMeasurement	Turns All Marker Interpolation ON and OFF for the measurement.
<u>putDataComplex</u>	IMeasurement	Puts complex data into one of five data buffers.
<u>putDataScalar</u>	IMeasurement	Puts formatted variant data into the measurement results buffer.
<u>SearchFilterBandwidth</u>	IMeasurement	Searches the domain with the current BW target.

Properties	Interface	Description
<u>ActiveMarker</u>	IMeasurement	Returns a handle to the Active Marker object.
<u>BalancedMeasurement</u>	IMeasurement	Sets the measurement type that is used with balanced topologies.

<u>BandwidthTarget</u>	IMeasurement	The insertion loss value at which the bandwidth of a filter is measured.
<u>BandwidthTracking</u>	IMeasurement	Turns Bandwidth Tracking function ON and OFF.
<u>CalibrationName</u>	IMeasurement2	Returns the name of the current cal type.
<u>CalibrationType</u>	IMeasurement	Set or get the calibration type for the measurement.
<u>CalibrationTypeID</u>	IMeasurement2	Sets or returns the current cal type to the Cal Set ID (CLSID).
<u>Center</u>	IMeasurement2	Returns the stimulus value of the center point for the measurement.
<u>channelNumber</u>	IIMeasurement	Returns the channel number. Shared with the Channel Object
<u>Domain</u>	IMeasurement2	Returns the domain (frequency, time, power) for the measurement.
<u>ElectricalDelay</u>	IMeasurement	Sets electrical delay.
<u>ElecDelayMedium</u>	IMeasurement2	Sets or returns the characteristic of the electrical delay medium.
<u>ErrorCorrection</u>	IMeasurement	Set or get the state of error correction for the measurement.
<u>FilterBW</u>	IMeasurement	Returns the results of the SearchBandwidth method.
<u>FilterCF</u>	IMeasurement	Returns the Center Frequency result of the SearchBandwidth method.
<u>FilterLoss</u>	IMeasurement	Returns the Loss value of the SearchBandwidth method.
<u>FilterQ</u>	IMeasurement	Returns the Q (quality factor) result of the SearchBandwidth method.
<u>Format</u>	IMeasurement	Sets display format.
<u>Gating</u>	IMeasurement	Controls Time Domain Gating.
<u>InterpolateCorrection</u>	IMeasurement	Turns ON and OFF the calculation of new error terms when stimulus values change.
<u>InterpolateNormalization</u>	IMeasurement	Turns ON and OFF normalization interpolation when stimulus values change after receiver power cal of unratiod measurements.
<u>IsSparameter</u>	IMeasurement2	Returns true if measurement represents an S-Parameter.
<u>LimitTest</u>	IMeasurement	Collection for iterating through the Limit Segment objects (Limit Lines).
<u>LimitTestFailed</u>	IMeasurement	Returns the results of limit testing

<u>LoadPort</u>	IMeasurement	Returns the load port number associated with an S-parameter reflection measurement.
<u>LogMagnitudeOffset</u>	IMeasurement	Sets or returns the value that normalized, unratiod, receiver power measurement data will be shifted by
<u>MagnitudeOffset</u>	IMeasurment4	Offsets the magnitude of the entire data trace to a specified value.
<u>MagnitudeSlopeOffset</u>	IMeasurment4	Offsets the magnitude of the data trace to a value that changes linearly with frequency.
<u>Marker</u>	IMeasurement	Contains the methods and properties that control Markers.
<u>MarkerFormat</u>	IMeasurement	Sets or returns the format of all the markers in the measurement.
<u>Marker State</u>	IMeasurement3	Sets or returns the ON / OFF state of a marker.
<u>Mean</u>	IMeasurement	Returns the mean value of the measurement.
<u>Name</u>	IMeasurement	Sets or returns the name of the measurement.
<u>NAWindow</u>	IMeasurement	Controls the part of the display that contains the graticule, or what is written on the display.
<u>Normalization</u>	IMeasurement	Turns ON or OFF normalization for receiver power cal of unratiod measurements
<u>Number</u>	IMeasurement	Returns the number of the measurement.
<u>NumberOfPoints</u>	IMeasurement2	Returns the Number of Points of the measurement.
<u>Parameter</u>	IMeasurement	Returns the measurement Parameter.
<u>PeakToPeak</u>	IMeasurement	Returns the Peak to Peak value of the measurement.
<u>PhaseOffset</u>	IMeasurement	Sets the Phase Offset for the active channel.
<u>ReceivePort</u>	IMeasurement2	Returns the receiver port of the measurement.
<u>ReferenceMarkerState</u>	IMeasurement	Turns the reference marker ON or OFF
<u>ShowStatistics</u>	IMeasurement	Displays and hides the measurement statistics (peak-to-peak, mean, standard deviation) on the screen.
<u>Smoothing</u>	IMeasurement	Turns ON and OFF data smoothing.
<u>SmoothingAperture</u>	IMeasurement	Specifies or returns the amount of smoothing as a ratio of the number of data points in the measurement trace.
<u>SourcePort</u>	IMeasurement2	Returns the source port of the measurement.
<u>Span</u>	IMeasurement2	Returns the stimulus span (stop - start) for the measurement.

<u>StandardDeviation</u>	IMeasurement	Returns the standard deviation of the measurement.
<u>Start</u>	IMeasurement2	Returns the stimulus value of the first point for the measurement.
<u>StatisticsRange</u>	IMeasurement	Sets the User Range number for calculating measurement statistics.
<u>Stop</u>	IMeasurement2	Returns the stimulus value of the last point for the measurement.
<u>Trace</u>	IMeasurement	Controls scale, reference position, and reference line.
<u>TraceMath</u>	IMeasurement	Performs math operations on the measurement object and the trace stored in memory.
<u>Transform</u>	IMeasurement	Controls Time Domain transforms.
<u>View</u>	IMeasurement	Sets (or returns) the type of trace displayed on the screen
<u>WGCutoffFreq</u>	IMeasurement2	Sets or returns the value of the waveguide cut off frequency

IMeasurement History

Interface	Introduced with PNA Rev:
IMeasurement	1.0
IMeasurement2	3.0
IMeasurement3	4.0
IMeasurement4	4.2
IMeasurement5	5.0

IArrayTransfer Interface

Description

Contains methods for putting data in and getting data out of the analyzer using typed data. This interface transfers data more efficiently than the IMeasurement Interface.

Methods	Description
<u>getComplex</u>	Retrieves real and imaginary data from the specified buffer.
<u>getNAComplex</u>	Retrieves typed NAComplex data from the specified buffer.
<u>getPairedData</u>	Retrieves magnitude and phase data pairs from the specified buffer.
<u>getScalar</u>	Retrieves scalar data from the specified buffer.
<u>putComplex</u>	Puts real and imaginary data into the specified buffer.
<u>putNAComplex</u>	Puts typed NAComplex data into the specified buffer.
<u>putScalar</u>	Puts scalar data into the measurement result buffer.

Properties	Description
None	

IArrayTransfer History

Interface	Introduced with PNA Rev:
IArrayTransfer	1.0

Measurement Collection

Description

A collection object that provides a mechanism for iterating through the Application measurements.

Accessing the Measurements collection

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim measments As Measurements
Set measments = app.Measurements
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Description
Add	Adds a Measurement to the collection.
Item	Use to get a handle on a measurement in the collection.
Remove	Removes a measurement from the measurements collection.

Properties	Description
Count	Returns the number of measurements in the analyzer.
Parent	Returns a handle to the current Application.



NAWindow Object

Description

The NAWindow object controls the part of the display that contains the graticule, or what is written on the display.

Accessing the NaWindow object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim window As NAWindow
Set window = app.NAWindows(1)
window.AutoScale
```

or

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", "analyzerName")


app.NAWindows(1).AutoScale
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

(**Bold** Methods or Properties provide access to a child object)

Methods	Description
Autoscale	Autoscales all measurements in the window. Shared with the Trace Object
ShowMarkerReadout	Shows and Hides the Marker readout for the active marker in the upper-right corner of the window object.
 ShowTable	Shows or Hides the specified table for the active measurement in the lower part of the window object.

Properties	Description
ActiveTrace	Sets a trace to the Active Trace.
MarkerReadout	Sets and reads the state of the Marker readout for the active marker in the upper-right corner of the window object.
MarkerReadoutSize	Specifies the size of font used when displaying Marker readout in the selected window.
OneMarkerReadoutPerTrace	Either show marker readout of only the active trace or all of the traces simultaneously.

<u>Title</u>	Writes or reads a custom title for the window.
<u>TitleState</u>	Turns ON and OFF the window title.
<u>Trace</u>	Collection for getting a handle to a trace or iterating through the traces in a window.
<u>WindowNumber</u>	Reads the number of the active window.
<u>WindowState</u>	Maximizes or minimizes a window. Shared with the Application Object

INaWindow History

Interface	Introduced with PNA Rev:
INaWindow	1.0

NAWindows Collection

Description

A collection object that provides a mechanism for iterating through the Application windows.

Accessing the NaWindows collection

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim windows As NAWindows
Set windows = app.NAWindows
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Description
Add	Adds a window to the NAWindows collection.
Item	Use to get a handle to a window in the collection.
Remove	Removes a window from the NAWindows collection.

Properties	Description
Count	Returns the number of windows on the analyzer.
Parent	Returns a handle to the current Application.



PortExtension Object OBSOLETE

ALL methods and properties on the PortExtension Object are Obsolete. Instead, use the port extension properties of the [Fixturing Object](#).

Description

Contains the methods and properties that control Port Extensions.

Accessing a PortExtension object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim PortExt As PortExtension
Set PortExt = app.PortExtension
```

See Also:

[PNA Automation Interfaces](#)


[The PNA Object Model](#)

Methods

None

Property

Description

Input A	Sets the Input A extension value.
Input B	Sets the Input B extension value.
Input C	Sets the Input C extension value.
 Port 1	Sets the Port 1 extension value.
Port 2	Sets the Port 2 extension value.
Port 3	Sets the Port 3 extension value.
State	Turns Port Extensions ON and OFF.

IPort Extension History

Interface	Introduced with PNA Rev:
IPort Extension	1.0

PowerLossSegment Object

Description

Contains the properties describing a segment of the power loss table used in source power calibration.

You can get a handle to one of these segments through the [segments.Item](#) Method of the PowerLossSegments collection.

Accessing the PowerLossSegment object

You can get a handle to one of these segments through `PowerLossSegments.Item(n)`

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim PwrLossSeg As PowerLossSegment
Set PwrLossSeg = app.SourcePowerCalibrator.PowerLossSegments(1)
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods

None

Properties

Description

[Frequency](#)

The frequency (Hz) associated with this segment.
Shared with the PowerSensorCalFactorSegment Object

 [ss](#)

The loss value (dB) associated with this segment.

[SegmentNumber](#)

Returns the number of this segment
Shared with the PowerSensorCalFactorSegment Object

IPowerLossSegment History

Interface	Introduced with PNA Rev:
IPowerLossSegment	2.0

PowerLossSegments Collection

Description

A collection object that provides a mechanism for iterating through the segments of the power loss table used in source power calibration.

Accessing the PowerLossSegments collection

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim PwrLossSegs As PowerLossSegments
Set PwrLossSegs = app.SourcePowerCalibrator.PowerLossSegments
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Description
Add	Adds a PowerLossSegment object to the collection.
Item	Use to get a handle to a PowerLossSegment object in the collection.
Remove	Removes an object from the collection.

Properties	Description
Count	Returns the number of objects in the collection.
Parent	Returns a handle to the Parent object (SourcePowerCalibrator) of this collection.



PowerSensor Object

Description

Each power sensor connected to the power meter associated with Source Power Calibration will have a PowerSensor object created to represent it. These PowerSensor objects reside in the [PowerSensors](#) collection within the SourcePowerCalibrator object. You cannot directly create PowerSensor objects, but can only retrieve existing ones from the PowerSensors collection.

The PowerSensorCalFactorSegment object is also accessed through the PowerSensor object. These are accessed through the CalFactorSegments collection in the PowerSensor object.

Accessing a PowerSensor object

```
Dim pna As AgilentPNA835x.Application
Set pna = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim powerCalibrator as SourcePowerCalibrator
Dim powerSensor as PowerSensor
Dim calFactorSegment as PowerSensorCalFactorSegment

Set powerCalibrator = pna.SourcePowerCalibrator

' Specify GPIB address of the power meter.
powerCalibrator.PowerMeterGPIBAddress = 13

' Each time the PowerSensors collection is accessed, the power meter is queried to
determine which channels have sensors attached. The collection is updated
accordingly.

If powerCalibrator.PowerSensors.Count > 0 Then
' If channel B of the meter has a sensor attached but channel A does not, then
element 1 of the
' collection is sensor B. Whenever channel A has a sensor, sensor A will be element
1.
Set powerSensor = powerCalibrator.PowerSensors(1)
' Insert one new PowerSensorCalFactorSegment at the beginning of the collection
(index 1).

powerSensor.CalFactorSegments.Add(1)
' Assign our variable to refer to that object.
Set calFactorSegment = powerSensor.CalFactorSegments(1)

' Set property values for that object.
calFactorSegment.Frequency = 300000
' frequency in Hz
calFactorSegment.CalFactor = 98
' cal factor in percent

End If
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

(**Bold** Methods or Properties provide access to a child object)

Methods	Description
---------	-------------

None

Properties	Description
------------	-------------

<u>CalFactorSegments</u>	Collection for iterating through the segments of a power sensor cal factor table.
<u>MinimumFrequency</u>	Minimum usable frequency (Hz) specified for this power sensor.
<u>MaximumFrequency</u>	Maximum usable frequency (Hz) specified for this power sensor.
<u>PowerMeterChannel</u>	Identifies which power sensor this object corresponds to (or which channel of the power meter the sensor is connected to).
<u>ReferenceCalFactor</u>	Reference cal factor (%) associated with this power sensor.

IPowerSensor History

Interface	Introduced with PNA Rev:
IPowerSensor	2.0

PowerSensorCalFactorSegment Object

Description

Contains the properties describing a segment of a power sensor cal factor table.

Accessing the PowerSensorCalFactorSegment object

You can get a handle to one of these segments through [CalFactorSegments.Item\(n\)](#)

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim calFactSeg As CalFactorSegments
Set calFactSeg = app.SourcePowerCalibrator.Powersensors(1).CalFactorSegments(1)
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods

None

Properties

Description

[Frequency](#)

The frequency (Hz) associated with this segment.
Shared with the PowerLossSegment Object

[CalFactor](#)

The cal factor (%) associated with this segment.

[SegmentNumber](#)

Returns the number of this segment.

Shared with the PowerLossSegment Object



IPowerSensorCalFactorSegment History

Interface	Introduced with PNA Rev:
IPowerSensorCalFactorSegment	2.0

PowerSensors Collection

Description

A collection object that provides a mechanism for iterating through the PowerSensor objects which are connected to the power meter. Each time this collection object is accessed, the power meter is queried to determine how many sensors are connected to it. The collection size and order of objects is then adjusted accordingly before the requested method or property operation is performed. The power meter is specified by using the [PowerMeterGPIBAddress](#) property of the [SourcePowerCalibrator](#) object.

Accessing the PowerSensors Collection

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim PwrSensors As PowerSensors
Set PwrSensors = app.SourcePowerCalibrator.PowerSensors
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Description
Item	Use to get a handle to a PowerSensor object in the collection.
Properties	Description
Count	Returns the number of objects in the collection.
Parent	Returns a handle to the Parent object (SourcePowerCalibrator) of this collection.



Preferences Object

Description

Sets the preferences for saving citifiles.

Accessing the Preferences object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim pref As Preferences
Set pref = app.Preferences
```

See Also:

[Citifile Define Data Saves](#)

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods

None

Properties Description

[CitiContents](#) Specifies the contents of subsequent citifile saves.

[CitiFormat](#) Specifies the format of subsequent citifile saves.

[SnPFormat](#) Specifies the format of subsequent .S1P, .S2P, .S3P file saves.

IPreferences History

Interface	Introduced with PNA Rev:
IPreferences	4.0

SCPIStringParser Object

Description

Provides the ability to send a SCPI command from within the COM command.

Accessing the Port Extension object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim SCPI As IScpiStringParser
Set SCPI = app.ScpiStringParser
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods	Interface	Description
Parse	IScpiStringParser	Provides the ability to send a SCPI command from within the COM command.
Execute	IScpiStringParser2	Does not convert scpi errors. Use :SYST:ERR?

Properties

None

History

Interface	Introduced with PNA Rev:
IScpiStringParser	1.0
IScpiStringParser2	3.0

Segment Object

Description

Contains the methods and properties that affect a sweep segment.

Note: All of these properties are shared with at least one of the following objects: Channel, Cal Set, PowerSensorCalFactorSegment, or PowerLossSegment.

Accessing a Segment object

You can get a handle to a sweep segment through the segments collection.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim segs As ISegments
Set segs = app.ActiveChannel.Segments

segs(2).NumberOfPoints = 30
```

See Also:


[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Segment Sweep](#)

Methods

None

Properties	Interface	Description
<u>centerFrequency</u>	ISegment	Sets or returns the center frequency of the segment. Shared with the Channel Object
 <u>DwellTime</u>	ISegment	Dwell time value. Shared with the Channel Object
<u>FrequencySpan</u>	ISegment	Sets or returns the frequency span of the segment. Shared with the Channel Object
<u>IFBandwidth</u>	ISegment	Sets or returns the IF Bandwidth of the segment. Shared with the Channel Object and Cal Set object.
<u>NumberOfPoints</u>	ISegment	Sets or returns the Number of Points of the segment. Shared with the Channel Object
<u>SegmentNumber</u>	ISegment	Returns the number of the current segment.

<u>StartFrequency</u>	ISegment	Sets or returns the start frequency of the segment. Shared with the Channel Object
<u>State</u>	ISegment	Turns On or OFF a segment.
<u>StopFrequency</u>	ISegment	Sets or returns the stop frequency of the segment. Shared with the Channel Object
<u>TestPortPower</u>	ISegment	Sets or returns the RF power level of the segment. Shared with the Channel Object

ISegment History

Interface	Introduced with PNA Rev:
ISegment	1.0

Segments Collection

Description

A collection object that provides a mechanism for iterating through the sweep segments of a channel. Sweep segments are a potentially faster method of sweeping the analyzer through only the frequencies of interest. Learn more about [Segment Sweep](#).

Accessing the Segments collection

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim segs As ISegments
Set segs = app.ActiveChannel.Segments
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	Interface See History	Description
Add	ISegments	Adds an item to either the Segments collection.
Item	ISegments	Use to get a handle to a segment in the collection..
Remove	ISegments	Removes an item from a collection of objects.
SetAllSegments	ISegments2	Uploads a segment table to the PNA.

Properties		Description
LowArbitrarySegments	ISegments3	Enables the setup of arbitrary segment sweep
Count	ISegments	Returns the number of items in a collection of objects.
IF Bandwidth Option	ISegments	Enables the IFBandwidth to be set on individual sweep segments.
Parent	ISegments	Returns a handle to the current naNetworkAnalyzer application..
Source Power Option	ISegments	Enables setting the Source Power for a segment.

ISegments History

Interface	Introduced with PNA Rev:
------------------	---------------------------------

ISegments	1.0
-----------	-----

ISegments2	3.5
------------	-----

ISegments3	4.2
------------	-----

SMCType Object

Description

Contains the methods and properties to perform an Scalar Measurement Calibration for the Frequency Converter Application (option 083).

Accessing the SMCType object

See an example which [creates and calibrates an SMC measurement](#).

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods

AcquireStep	Acquire the measurement data for the specified step in the calibration process.
GenerateErrorTerms	Generates the error terms for the calibration.
GenerateSteps	Returns the number of steps required to complete the calibration.
GetStepDescription	Returns the description of the specified step calibration process.
Initialize	Begins a calibration.

Properties

Description

AutoOrient	Sets ECAL module automatic orientation ON or OFF.
CalibrationPort	Sets or returns the calibration source port for the calibration.
CalKitType	Sets and returns a calibration kit type for calibration.
CompatibleCalKits	Returns a list of cal kits that are compatible with the connector type for the specified port.
ConnectorType	Sets or queries the connector type for the specified port.
Do2PortEcal	Specify ECAL or Mechanical calibration.
EcalCharacterization	Specifies the characterization data within an ECal module to be used for the calibration.

<u>EcalOrientation</u>	Specifies which port of the ECal module is connected to which port of the PNA when the AutoOrient property = False.
<u>OmitIsolation</u>	Sets and returns whether Isolation portion of the calibration will be performed or not.
<u>ThruCalMethod</u>	Sets and returns the method for performing the thru portion of the calibration.
<u>ValidConnectorTypes</u>	Returns a list of connector types for which there are calibration kits.

ISMCType History

Interface	Introduced with PNA Rev:
ISMCType	3.5

SourcePowerCalibrator Object

Description

This object is a child of the Application object and is a vehicle for performing source power calibrations.

Accessing the SourcePowerCalibrator Object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim ispc As ISourcePowerCalibrator
Set ispc = app.SourcePowerCalibrator
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Note: Interface **ISourcePowerCalibrator** is abbreviated as **ISPC** in the following table.

(**Bold** Methods or Properties provide access to a child object)

Methods	Interface	Description
	See History	
AbortPowerAcquisition	ISPC	Aborts a source power cal acquisition sweep that is currently in progress.
AcquirePowerReadings	ISPC	Initiates a source power cal acquisition.
ApplyPowerCorrectionValues	ISPC	Applies correction values after completing a source power cal acquisition sweep.
CheckPower	ISPC2	Measures power at a specific frequency. Used to test power level before and/or after applying a source power calibration.
LaunchPowerMeterSettingsDialog	ISPC2	Launches the Power Meter Settings dialog on the PNA.
SetCallInfo	ISPC	OBSOLETE
SetCallInfo2	ISPC3	REPLACEMENT - Specifies the type of source power calibration about to be performed.
SetPowerAcquisitionDevice	ISPC3	Sets the power sensor channel (A or B) to be used. This method is ONLY necessary when performing an SMC calibration.

Properties	Interface	Description
------------	-----------	-------------

<u>CalPower</u>	ISPC	Specifies the power level that is expected at the desired reference plane.
<u>IterationsTolerance</u>	ISPC3	Sets the maximum desired deviation from the sum of the test port power and the offset value.
<u>MaximumIterationsPerPoint</u>	ISPC3	Specifies maximum number of readings to take at each data point for iterating the source power.
<u>PowerAcquisitionDevice</u>	ISPC2	Specifies the power sensor channel (A or B) that is currently selected for use at a specific frequency.
<u>PowerLossSegments (collection)</u>	ISPC2	Collection for iterating through the segments of the power loss table used in source power calibration.
<u>PowerMeterGPIBAddress</u>	ISPC	Specifies the GPIB address of the power meter.
<u>PowerSensors (collection)</u>	ISPC2	Collection for iterating through the PowerSensor objects which are connected to the power meter for a source power cal.
<u>ReadingsPerPoint</u>	ISPC	Specifies the maximum power readings for power meter settling.
<u>ReadingsTolerance</u>	ISPC3	Power meter settling tolerance value.
<u>UsePowerLossSegments</u>	ISPC	Specifies if subsequent calls to the AcquirePowerReadings method will make use of the loss table (PowerLossSegments).
<u>UsePowerSensorFrequencyLimits</u>	ISPC	Specifies if subsequent calls to the AcquirePowerReadings method will make use of power sensor frequency checking capability.

ISourcePowerCalibrator History

Interface	Introduced with PNA Rev:
ISourcePowerCalibrator	2.0
ISourcePowerCalibrator2	3.5
ISourcePowerCalibrator3	4.0

Trace Object

Description

The Trace object controls how the measurement data is displayed. You can control scale, reference position, and value from the Trace Object.

Accessing a Trace object

There are several ways to get a handle to a trace.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)
```

```
Dim trace As Trace
```

Then you can do any of the following:

```
Set trace = app.NAWindows(1).traces(1)
```

```
set trace = app.NAWindows.item(1).ActiveTrace
```

```
set trace = app.ActiveNAWindow.traces.item(1)
```

```
set trace = app.ActiveNAWindow.ActiveTrace
```

```
Set trace = app.Measurements(1).trace
```

```
Set trace = app.ActiveMeasurement.trace
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Traces, Channels, and Windows on the PNA](#)

	Description
Methods	

[Autoscale](#) Autoscales the trace or all of the traces in the selected window.

 Shared with the NAWindow Object

	Description
Property	

[Name](#) Sets or returns the trace name

[ReferencePosition](#) Sets or returns the Reference Position of the active trace.

[ReferenceValue](#) Sets or returns the value of the Y-axis Reference Level of the active trace.

[YScale](#) Sets or returns the Y-axis Per-Division value of the active trace.

ITrace History

Interface

**Introduced with PNA
Rev:**

ITrace 1.0

Traces Collection

Description

Child of the **Application** Object. A collection that provides a mechanism for getting a handle to a trace or iterating through the traces in a window.

Accessing the Traces collection

Get a handle to the traces collection through the NaWindows collection. The following example sets the variable **trcs** to the collection of traces in window 1 of the NaWindows collection.

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)

Dim trcs As traces
Set trcs = app.NAWindows(1).traces
```

See Also:

[Collections in the Analyzer](#)

[The PNA Object Model](#)

Methods	
Methods	Description
Item	Use to get a handle to a trace

Properties	
Properties	Description
Count	Returns the number of traces in the collection.
Parent	Returns a handle to the current Application.

Transform Object

Description

Contains the methods and properties that control Time Domain transforms.

Accessing the Transform Object

```
Dim app As AgilentPNA835x.Application
Set app = CreateObject("AgilentPNA835x.Application", <analyzerName>)


Dim trans As Transform
Set trans = app.ActiveMeasurement.Transform
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Time Domain Topics](#)

Methods	Interface	Description
SetFrequencyLowPass	ITransform	Sets low frequencies for low pass.
Properties		Description
Center	ITransform	Sets or returns the Center time. Shared with the Gating Object
CoupledParameters	ITransform2	Select Transform parameters to couple
DistanceMarkerMode	ITransform2	Sets the measurement type in order to determine the correct marker distance.
DistanceMarkerUnit	ITransform2	Sets the unit of measure for the display of marker distance values.
 pulseWidth	ITransform	Sets or returns the Impulse Width of Time Domain transform windows.
KaiserBeta	ITransform	Sets or returns the Kaiser Beta of Time Domain transform windows.
Mode	ITransform	Sets the type of transform.
Span	ITransform	Sets or returns the Span time. Shared with the Gating Object
Start	ITransform	Sets or returns the Start time. Shared with the Gating Object
State	ITransform	Turns an Object ON and OFF.
StepRiseTime	ITransform	Sets or returns the Rise time of the stimulus in Low Pass Step Mode.

Stop

ITransform

Sets or returns the Stop time.
Shared with the Gating Object

ITransform History

Interface	Introduced with PNA Rev:
ITransform	1.0
ITransform2	4.2

TriggerSetup Object

Description

These properties setup Global triggering that effects the entire PNA application.

Accessing the TriggerSetup object

```
Dim app as AgilentPNA835x.Application
Dim trigSetup as ITriggerSetup
Set trigSetup = app.TriggerSetup
```

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

[Triggering in the PNA](#)

Methods	Interface	Description
	See History (below)	

None

Properties		Description
AcceptTriggerBeforeArmed	ITriggerSetup2	Allows a trigger signal to be remembered and then used when the PNA becomes armed (ready to be triggered).
ExternalTriggerConnectionBehavior	ITriggerSetup	Configures the external triggering signal for the PNA
Scope	ITriggerSetup	Determines whether a trigger signal affects a single channel or all channels in the PNA.
Source	ITriggerSetup	Sets or returns the source of triggering in the PNA.
TriggerOutputEnabled	ITriggerSetup2	Enables the PNA to send trigger signals out the rear-panel TRIGGER OUT connector.

ITriggerSetup History

Interface	Introduced with PNA Rev:
ITriggerSetup	4.0
ITriggerSetup2	4.2

VMC Type Object

Description

Contains the methods and properties to perform a Vector Measurement Calibration for the Frequency Converter Application (option 083).

Accessing the VMCType object

See an example which [creates and calibrates a VMC measurement](#).

See Also:

[PNA Automation Interfaces](#)

[The PNA Object Model](#)

Methods

AcquireStep	Acquire the measurement data for the specified step in the calibration process.
GenerateErrorTerms	Generates the error terms for the calibration.
GenerateSteps	Returns the number of steps required to complete the calibration.
GetStepDescription	Returns the description of the specified step in the calibration process.
Initialize	Begins a calibration.

Properties

Description

AutoOrient	Sets ECAL module automatic orientation ON or OFF.
CalKitType	Sets and returns a calibration kit type for calibration.
CharacterizeMixerOnly	Sets and returns whether to perform a mixer characterization ONLY or full 2-port calibration.
CharFileName	Specifies the .S2P mixer characterization file name.
CharMixerReverse	Specifies the direction in which to characterize the calibration mixer.
CompatibleCalKits	Returns a list of cal kits that are compatible with the connector type for the specified port.
ConnectorType	Sets or queries the connector type for the specified port.
Do1PortEcal	Specify ECAL or Mechanical calibration for the mixer characterization portion of a VMC calibration.

<u>Do2PortEcal</u>	Specify ECAL or Mechanical calibration for the 2-port calibration portion of a VMC calibration.
<u>EcalCharacterization</u>	Specifies the characterization data within an ECal module to be used for the calibration.
<u>EcalOrientation1Port</u>	For Mixer Characterization ONLY - Specifies which port of the ECal module is connected to which port of the PNA
<u>EcalOrientation2Port</u>	For full 2-port VMC cal - Specifies which port of the ECal module is connected to which port of the PNA
<u>LoadCharFromFile</u>	Specifies and loads a mixer characterization (S2P) file.
<u>OmitIsolation</u>	Sets and returns whether Isolation portion of the calibration will be performed or not.
<u>ThruCalMethod</u>	Sets and returns the method for performing the thru portion of the calibration.
<u>ValidConnectorTypes</u>	Returns a list of connector types for which there are calibration kits.

IVMCType History

Interface	Introduced with PNA Rev:
IVMCType	3.5

AcceptTriggerBeforeArmed Property

Description Determines what happens to an EDGE trigger signal if it occurs before the PNA is ready to be triggered. (LEVEL trigger signals are always ignored.) For more information, see [External triggering](#).

VB Syntax `trigsetup.AcceptTriggerBeforeArmed = boolean`

Variable (Type) - Description

trigsetup A [TriggerSetup2](#) (**object**)

boolean Choose from:

0 - False - A trigger signal is ignored if it occurs before the PNA is ready to be triggered.

1 - True - A trigger signal is remembered and then used when the PNA becomes armed (ready to be triggered). The PNA remembers only one trigger signal.

Return Type Boolean

Default False

Examples `trigsetup.AcceptTriggerBeforeArmed = 1 'Write`

`atba = trigsetup.AcceptTriggerBeforeArmed 'Read`

C++ Syntax HRESULT get_AcceptTriggerBeforeArmed(BOOL *pVal);
HRESULT put_AcceptTriggerBeforeArmed(BOOL newVal);

Interface ITriggerSetup2

AcquisitionDirection Property

Description Specifies the direction of each part of a 2-port calibration.

VB Syntax `cal.AcquisitionDirection = value`

Variable (Type) - Description

cal A Calibrator **(object)**

value **(enum NADirection)** - Choose from:

0 - naForward - measures the forward direction

1 - naReverse - measures the reverse direction

Return Type Long Integer

Default naForward

Examples `cal.AcquisitionDirection = naForward`

C++ Syntax HRESULT AcquisitionDirection(tagNADirection dir);

Interface ICalibrator

Read-only

ActiveCalKit Property

Description	Returns a handle to the Active CalKit object. You can either (1) use the handle directly to access CalKit properties and methods, or (2) set a variable to the CalKit object. The variable retains a handle to the original object if another CalKit becomes active.
VB Syntax	1) <code>app.ActiveCalKit.<setting></code> or 2) <code>Set cKit = app.ActiveCalKit</code>
Variable	(Type) - Description
<code>app</code>	An Application (object)
<code><setting></code>	A CalKit property (or method) and arguments
<code>cKit</code>	(object) - A CalKit object
Return Type	CalKit object
Default	None
Examples	<pre>Public cKit as calKit Set cKit = app.ActiveCalKit 'read</pre>
C++ Syntax	HRESULT get_ActiveCalKit (ICalKit * kit)
Interface	IApplication

ActiveChannel Property

Description	Returns a handle to the Active Channel object. You can either (1) use the handle directly to access channel properties and methods, or (2) set a variable to the channel object. The variable retains a handle to the original channel if another channel becomes active.
VB Syntax	(1) <code>app.ActiveChannel.<setting></code> or (2) <code>Set chan = app.ActiveChannel</code>
Variable	(Type) - Description
<code>chan</code>	A Channel (object)
<code>app</code>	An Application (object)
<code><setting></code>	A channel property (or method) and arguments
Return Type	Channel object
Default	Not applicable
Examples	<pre>1) app.ActiveChannel.Averaging = 1 2) Public chan as Channel Set chan = app.ActiveChannel</pre>
C++ Syntax	<code>HRESULT get_ActiveChannel(IChannel* *pVal)</code>
Interface	<code>IApplication</code>

ActiveMarker Property

Description	Returns a handle to the Active Marker object. You can either (1) use the handle directly to access Marker properties and methods, or (2) set a variable to the Marker object. The variable retains a handle to the original object if another Marker becomes active.
VB Syntax	1) <i>meas.ActiveMarker.<setting></i> or 2) Set <i>mark</i> = <i>meas.ActiveMarker</i>
Variable	<u>(Type)</u> - Description
<i>meas</i>	(object) - An Measurement object
<i><setting></i>	A marker property (or method) and arguments
<i>mark</i>	(object) - A marker object
Return Type	marker object
Default	None
Examples	<pre>Public mark as marker Set mark = meas.ActiveMarker</pre>
<u>C++</u> Syntax	HRESULT get_ActiveMarker(IMarker** marker)
Interface	IMeasurement

Read-only

ActiveMeasurement Property

Description	Returns a handle to the Active Measurement object. You can either (1) use the handle directly to access measurement properties and methods, or (2) set a variable to the measurement object. The variable retains a handle to the original measurement.
VB Syntax	1) <code>app.ActiveMeasurement.<setting></code> or 2) Set <code>meas = app.ActiveMeasurement</code>
Variable	(Type) - Description
<code>meas</code>	A Measurement (object)
<code>app</code>	An <u>Application</u> (object)
<code><setting></code>	A measurement property (or method) and arguments
Return Type	Measurement object
Default	None
Examples	<pre>1) app.ActiveMeasurement.Averaging = 1 2) Public meas as Measurement Set meas = app.ActiveMeasurement</pre>
C++ Syntax	HRESULT get_ActiveMeasurement(IMeasurement **ppMeas)
Interface	IApplication

ActiveNAWindow Property

Description Returns a handle to the Active Window object. You can either **(1)** use the handle directly to access window properties and methods, or **(2)** set a variable to the window object. The variable retains a handle to the original window if another window becomes active.

VB Syntax 1) `app.ActiveNAWindow.<setting>`
or
2) Set `win = app.ActiveNAWindow`

Variable (Type) - Description

`win` A NAWindow **(object)**

`app` An Application **(object)**

`<setting>` A NAWindow property (or method) and arguments

Return Type A NAWindow object

Default Not applicable

Examples

```
Public win as NAWindow
Set win = app.ActiveWindow
```

C++ Syntax HRESULT get_ActiveNAWindow(INAWindow **ppWindow)

Interface IApplication

ActiveXAxisRange Property

Description Sets or returns the swept parameter to display on the X-axis for the selected FCA measurement.

VB Syntax `mixer.ActiveXAxisRange = value`

Variable **(Type) - Description**

mixer A Mixer **(object)**

value **(Enum as MixerStimulusRange)** - Parameter to display on the X-axis. Choose from:

0 - mixINPUT - Input frequency span

1 - mixOUTPUT - Output frequency span

2 - mixLO_1 - First LO frequency span

3 - mixLO_2 - Second LO frequency span

Return Type Enum

Default OUTPUT

Examples

```
mixer.ActiveXAxisRange = 1 'Write
variable = mixer.ActiveXAxisRange 'Read
```

C++ Syntax HRESULT get_ActiveXAxisRange(tagMixerStimulusRange *Val)
 HRESULT put_ActiveXAxisRange(tagMixerStimulusRange newVal)

Interface IMixer3

ActiveTrace Property

Description Returns a handle to the Active Trace object. You can either **(1)** use the handle directly to access trace properties and methods, or **(2)** set a variable to the trace object. The variable retains a handle to the original trace if another trace becomes active.

VB Syntax 1) `win.ActiveTrace.<setting>`
or
 2) Set `trce = win.ActiveTrace`

Variable (Type) - Description

`trce` A Trace **(object)**

`win` An NAWindow **(object)**

`<setting>` A trace property (or method) and arguments

Return Type An NAWindow object

Default None

Examples

```
1) win.ActiveTrace.Autoscale
2) Public trce as Trace
   Set trce = Application.ActiveNAWindow.ActiveTrace
```

C++ Syntax HRESULT get_ActiveTrace(ITrace* *pVal)

Interface INAWindow

Write/Read

AllowArbitrarySegments Property

Description Enables you to setup a segment sweep with arbitrary frequencies. The start and stop frequencies of each segment can overlap other segments. Also, each segment can have a start frequency that is greater than its stop frequency which causes a reverse sweep over that segment. Learn more about [Arbitrary Segment Sweep](#).

VB Syntax `segs.AllowArbitrarySegments = value`

Variable (Type) - Description

`segs` A [Segments](#) collection (**object**)

`value` (**boolean**)

True - Allows the setup of arbitrary segment sweep.

False - Prevents the setup of arbitrary segment sweep.

Return Type Boolean

Default False

Examples `segs.AllowArbitrarySegments = True 'Write`

`AllowArbSegs = AllowArbitrarySegments 'Read`

C++ Syntax HRESULT get_AllowArbitrarySegments(VARIANT_BOOL *pVal)
 HRESULT put_AllowArbitrarySegments(VARIANT_BOOL newVal)

Interface ISegments3

AlternateSweep Property

Description Sets sweeps to either alternate or chopped.

VB Syntax *object*.AlternateSweep = *value*

Variable (Type) - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

value (**boolean**) - Choose either:

False (0) - Sweep mode set to **Chopped** - reflection and transmission are measured on the same sweep.

True (1) - Sweep mode set to **Alternate** - reflection and transmission measured on separate sweeps. Improves Mixer bounce and Isolation measurements. Increases cycle time.

Return Type boolean

Default False (0)

Examples `chan.AlternateSweep = True 'Write`

`altSwp = chan.AlternateSweep 'Read`

C++ Syntax HRESULT AlternateSweep(VARIANT_BOOL *pVal)
HRESULT AlternateSweep(VARIANT_BOOL newVal)

Interface IChannel
ICalSet3

Read-only

Application Property

Description Returns the name of the Analyzer making measurements on the channel.

VB Syntax `chan.Application`

Variable **(Type) - Description**

`chan` A Channel (**object**)

Return Type object

Default None

Examples `rfna = chan.Application 'returns the Analyzer name`

C++ Syntax HRESULT get_Application(IApplication** Application)

Interface IChannel

Write/Read

ArrangeWindows Property

Description Sets or returns the arrangement of all the windows. Overlay, Stack2, Split3 and Quad4 will create windows.

To control the state of the one window you have a handle to, use [app.WindowState](#).

VB Syntax `app.ArrangeWindows = value`

Variable **(Type) - Description**

`app` An [Application](#) (**object**)

`value` (**enum NAWindowModes**) - Choose from:

0 - naTile

1 - naCascade

2 - naOverlay

3 - naStack2

4 - naSplit3

5 - naQuad4

Return Type NAWindowModes

Default naTile

Examples `app.ArrangeWindow = naTile 'Write`

`arrWin = app.ArrangeWindows 'Read`

C++ Syntax HRESULT put_ArrangeWindows(tagNAWindowModes newVal)

Interface IApplication

AttenuatorMode Property

Description Sets or returns the mode of operation of the attenuator control for the specified port number. This command is automatically set to Manual when an Attenuator value is set.

VB Syntax *object*.AttenuatorMode(*portNum*) = *value*

Variable (Type) - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

portNum (**long**) - Port number (1 or 2) of attenuator control to be changed.

value (**enum NAModes**) - Choose from:

0 - naAuto - Attenuator control set to automatic. The analyzer will set the attenuator control appropriately to deliver the specified power at the source.

1 - naManual - Specify the attenuator setting using chan.Attenuator (which automatically sets AttenuatorMode = naManual).

Return Type NAModes

Default 0 - Auto

Examples `chan.AttenuatorMode(1) = naAuto 'Write`

`attn = chan.AttenuatorMode(1) 'Read`

C++ Syntax HRESULT get_AttenuatorMode(long port, tagNAModes* pVal)
HRESULT put_AttenuatorMode(long port, tagNAModes newVal)

Interface IChannel
ICalSet3

Attenuator Property

Description Sets or returns the value of the attenuator control for the specified port number. Sending this command automatically sets AttenuatorMode to Manual.

VB Syntax *object*.Attenuator(*portNum*) = *value*

Variable (Type) - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

portNum (**long integer**) - Port number (1 or 2) of attenuator control to be changed.

value (**double**) - Attenuator value in dB in 10dB steps.

Note: To determine the maximum attenuator value, use MaximumSourceStepAttenuator Property

If an invalid value is entered, the analyzer will select the next lower valid value. For example, if 19.9 is entered the analyzer will select 10 dB attenuation.

Return Type Double

Default 20 dB

Examples `chan.Attenuator(1) = 20 'Write`

`attn = chan.Attenuator(cnum) 'Read`

C++ Syntax HRESULT get_Attenuator(long port, double *pVal)
HRESULT put_Attenuator(long port, double newVal)

Interface IChannel
ICalSet3

AutoOrient Property

Description Sets ECAL module automatic orientation ON or OFF.

VB Syntax *obj.AutoOrient = bool*

Variable **(Type) - Description**

obj SMCType (object)

or

VMCType (object)

bool (Boolean)

1 - Set AutoOrientation ON

0 - Set AutoOrientation OFF

Return Type Boolean

Default 1

Examples `Smc.AutoOrient = 1`

C++ Syntax HRESULT put_AutoOrient(VARIANT_BOOL bAutoOrient);

HRESULT get_AutoOrient(VARIANT_BOOL *bAutoOrient);

Interface SMCType

VMCType

AutoPortExtConfig Property

Description Sets the frequency span that is used to calculate Automatic Port Extension. [Learn more about calculating Automatic Port Extension.](#)

VB Syntax `fixture.AutoPortExtConfig = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`value` (ENUM as NAAutoPortExtConfig)

0 naAPEC_CSPN - Use current span.

1 naAPEC_AMKR - Use active marker frequency.

2 naAPEC_USPN - Use custom user span. Use [AutoPortExtSearchStart Property](#) and [AutoPortExtSearchStop Property](#) to specify start and stop frequency.

Return Type ENUM

Default **0 naAPEC_CSPN**

Examples `fixture.AutoPortExtConfig = naAPEC_AMKR`

`value = fixture.AutoPortExtConfig 'Read`

C++ Syntax `HRESULT get_AutoPortExtConfig(tagNAAutoPortExtConfig *pVal);`
`HRESULT put_AutoPortExtConfig(tagNAAutoPortExtConfig Val);`

Interface IFixturing2

AutoPortExtDCOffset Property

Description Specifies whether or not to include DC Offset as part of automatic port extension. Learn more about [Automatic DC Offset](#). Only allowed when [AutoPortExtLoss Property](#) is set to ON.

VB Syntax *fixture*.AutoPortExtDCOffset = *bool*

Variable **(Type) - Description**

fixture A [Fixturing](#) (**object**)

bool ON (or 1) - Includes DC Offset correction.

OFF (or 0) - Does NOT include DC Offset correction.

Return Type Boolean

Default OFF (or 0)

Examples `fixture.AutoPortExtDCOffset = 1`

```
value = fixture.AutoPortExtDCOffset 'Read
```

C++ Syntax HRESULT get_AutoPortExtDCOffset(VARIANT_BOOL *pState);
HRESULT put_AutoPortExtDCOffset(VARIANT_BOOL bState);

Interface IFixturing2

AutoPortExtLoss Property

Description Specifies whether or not to include loss correction as part of automatic port extension. [Learn more about Loss Compensation in port extension.](#)

VB Syntax *fixture*.AutoPortExtLoss = *bool*

Variable **(Type) - Description**

fixture A [Fixturing](#) (**object**)

bool ON (or 1) - Includes Loss correction.

OFF (or 0) - Does NOT include Loss correction.

Return Type Boolean

Default OFF (or 0)

Examples `fixture.AutoPortExtLoss = 1`

```
value = fixture.AutoPortExtLoss 'Read
```

C++ Syntax HRESULT get_AutoPortExtLoss(VARIANT_BOOL *pState);
HRESULT put_AutoPortExtLoss(VARIANT_BOOL bState);

Interface IFixturing2

AutoPortExtSearchStart Property

Description Set the start frequency for custom user span. Only applies when `fixture.AutoPortExtConfig = 0` **naAPEC_CSPN**.

[Learn more about User Span.](#)

VB Syntax `fixture.AutoPortExtSearchStart = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`value` (Double) User span start value. Must be within the frequency range of the active channel and less than the value set by [AutoPortExtSearchStop Property](#)

Return Type Double

Default Start frequency of the current active channel.

Examples `fixture.AutoPortExtSearchStart = 1E9`

```
value = fixture.AutoPortExtSearchStart 'Read
```

C++ Syntax HRESULT get_AutoPortExtSearchStart(double *pdVal);
HRESULT put_AutoPortExtSearchStart(double dVal);

Interface IFixturing2

AutoPortExtSearchStop Property

Description Set the stop frequency for custom user span. Only applies when `fixture.AutoPortExtConfig = 0 naAPEC_CSPN`.

[Learn more about User Span.](#)

Only applies when `fixture.AutoPortExtConfig = 0 naAPEC_CSPN`

VB Syntax `fixture.AutoPortExtSearchStop = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`value` (Double) User span stop value. Must be within the frequency range of the active channel and greater than the value set by [AutoPortExtSearchStart Property](#)

Return Type Double

Default Stop frequency of the current active channel.

Examples `fixture.AutoPortExtSearchStop = 1E9`

```
value = fixture.AutoPortExtSearchStop 'Read
```

C++ Syntax `HRESULT get_AutoPortExtSearchStop(double *pdVal);`
`HRESULT put_AutoPortExtSearchStop(double dVal);`

Interface IFixturing2

AutoPortExtState Property

Description Enables and disables automatic port extensions on the specified port. All enabled ports will have their reference plane automatically adjusted after performing Automatic Port Extension.

VB Syntax *fixture*.AutoPortExtState (*port*) = *bool*

Variable (Type) - Description

fixture A Fixturing (**object**)

port (**Integer**) Port number to enable or disable.

bool (Boolean)

False - Enables Auto Port Extensions

True - Disables Auto Port Extensions

**Return
Type** Boolean

Default OFF

Examples `fixture.AutoPortExtState(1) = 1`

`value = fixture.AutoPortExtState(2) 'Read`

C++ Syntax HRESULT get_AutoPortExtConfig(AutoPortExtState(short port, VARIANT_BOOL *pState);
HRESULT put_AutoPortExtConfig(AutoPortExtState(short port, VARIANT_BOOL bVal);

Interface IFixturing2

Read-only

AveragingCount Property

Description Returns the number of sweeps that have been acquired and averaged into the measurements on this channel. AveragingFactor specifies the number of sweeps to average. AveragingCount indicates the progress toward that goal.

VB Syntax *value* = *chan.AveragingCount*

Variable (Type) - Description

chan A Channel (**object**)

value (**Long Integer**) - Variable to store the returned count

Return Type Long Integer

Default Not Applicable

Example `avgcount = chan.AveragingCount`

C++ Syntax HRESULT get_AveragingCount(long* count)

Interface IChannel

Write/Read

AveragingFactor Property

Description	Specifies the number of measurement sweeps to combine for an average. Must also turn averaging ON by setting <code>chan.Averaging</code> = 1. Averaging is only allowed on ratioed measurements; not on single input measurements.
VB Syntax	<code>chan.AveragingFactor = value</code>
Variable	(Type) - Description
<code>chan</code>	A Channel (object)
<code>value</code>	(Long Integer) - Number of measurement sweeps to average. Choose any number between 1 and 1024 .
Return Type	Long Integer
Default	1
Examples	<pre>chan.AveragingFactor = 5 'Write</pre> <pre>avgfact = chan.AveragingFactor ' doesn't work -Read</pre>
C++ Syntax	<pre>HRESULT get_AveragingFactor(long *pVal) HRESULT put_AveragingFactor(long newVal)</pre>
Interface	IChannel

Averaging Property

Description Turns trace averaging ON or OFF for all measurements on the channel. Averaging is only allowed on ratioed measurements; not on single input measurements.

VB Syntax `chan.Averaging = state`

Variable **(Type) - Description**

`chan` A Channel **(object)**

`state` **(boolean)**
0 - Turns averaging OFF
1 - Turns averaging ON

Return Type Boolean

Default 0

Examples `chan.Average = 1 'Write`

`averg = chan.Averaging 'Read`

C++ Syntax HRESULT get_Averaging(BOOL *pVal)
HRESULT put_Averaging(BOOL newVal)

Interface IChannel

AvoidSpurs Property

Description Sets and returns the state of the avoid spurs feature.

VB Syntax `mixer.AvoidSpurs = boolean`

Variable **(Type) - Description**

mixer A Mixer **(object)**

value **(Boolean)** - State of avoid spurs feature. Choose from

0 Avoid spurs OFF

1 Avoid spurs ON

Return Type Boolean

Default 0

Examples

```
mixer.AvoidSpurs = 1 'Write  
variable = mixer.AvoidSpurs 'Read
```

C++ Syntax HRESULT get_AvoidSpurs(Bool *bVal)
HRESULT put_AvoidSpurs(Bool newVal)

Interface IMixer3

BalancedMode Property

Description Sets and returns whether the balanced transform is ON or OFF

VB Syntax *balMeas*.**BalancedMode** = *value*

Variable (Type) - Description

balMeas A BalancedMeasurement (**object**)

value (**Boolean**) - State of balanced transform. Choose from

0 Balanced Transform OFF

1 Balanced Transform ON

Return Type Boolean

Default 0

Examples `balMeas.BalancedMode = 1 'Write`

`variable = balMeas.BalancedMode 'Read`

C++ Syntax HRESULT get_BalancedMode(VARIANT_BOOL *bVal)

HRESULT put_BalancedMode(VARIANT_BOOL newVal)

Interface IBalancedMeasurement

Write/Read

BandwidthTarget Property

Description Sets the insertion loss value at which the bandwidth of a filter is measured (using [BandwidthTracking](#) or [SearchFilterBandwidth](#)). For example, if you want to determine the filter bandwidth 3 db below the bandpass peak value, set BandwidthTarget to **-3**.

VB Syntax *meas.BandwidthTarget = value*

Variable **(Type) - Description**

meas A Measurement (**object**)

value (**single**) - Target value. Choose any number between **-500** and **500**

Return Type Single

Default -3

Examples `meas.BandwidthTarget = -3 'Write`

`fbw = meas.BandwidthTarget 'Read`

C++ Syntax HRESULT put_BandwidthTarget(float target)
HRESULT get_BandwidthTarget(float* target)

Interface IMeasurement

BandwidthTracking Property

Description Searches continually (every sweep) for the current BandwidthTarget (default is -3). To search the filter bandwidth for ONE SWEEP only (not continually), use meas.SearchFilterBandwidth.

This feature uses markers 1-4. To turn off these markers, either turn them off individually or DeleteAllMarkers.

The bandwidth statistics are displayed on the analyzer screen. To get the bandwidth statistics, use either GetFilterStatistics or FilterBW, FilterCF, FilterLoss, or FilterQ.

The analyzer screen will show either Bandwidth statistics OR Trace statistics; not both.

To restrict the search to a UserRange with the bandwidth search, first activate marker 1 and set the desired UserRange. Then send the SearchFilterBandwidth command. The user range used with bandwidth search only applies to marker 1 searching for the max value. The other markers may fall outside the user range.

VB Syntax `meas.BandwidthTracking = value`

Variable (Type) - Description

`meas` A Measurement (**object**)

`value` (**boolean**)

1 - Turns bandwidth tracking ON

0 - Turns bandwidth tracking OFF

Return Type Boolean

Default 0 - OFF

Examples `meas.BandwidthTracking = 1 'Write`

`bwtrack = meas.BandwidthTracking 'Read`

C++ Syntax HRESULT put_BandwidthTracking(VARIANT_BOOL state)
HRESULT get_BandwidthTracking(VARIANT_BOOL* state)

Interface IMeasurement

BB_BalPort1Negative Property

Description With a Balanced - Balanced topology, returns the PNA port number that is connected to the Negative side of the DUT's logical Port 1.

Use [SetBBPorts Method](#) to set the port mapping for a Balanced - Balanced topology.

VB Syntax `var = balTopology.BB_BalPort1Negative`

Variable (Type) - Description

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

Return Type Long Integer

Default Not Applicable

Examples `variable = balTop.BB_BalPort1Negative 'Read`

C++ Syntax HRESULT get_BB_BalPort1Negative(long *bVal)

Interface IBalancedTopology

BB_BalPort1Positive Property

Description With a Balanced - Balanced topology, returns the PNA port number that is connected to the Positive side of the DUT's logical Port 1.

Use [SetBBPorts Method](#) to set the port mapping for a Balanced - Balanced topology.

VB Syntax `var = balTopology.BB_BalPort1Positive`

Variable (Type) - Description

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

Return Type Long Integer

Default Not Applicable

Examples `variable = balTop.BB_BalPort1Positive 'Read`

C++ Syntax HRESULT get_BB_BalPort1Positive(long *bVal)

Interface IBalancedTopology

BB_BalPort2Negative Property

Description With a Balanced - Balanced topology, returns the PNA port number that is connected to the Negative side of the DUT's logical Port 2.

Use [SetBBPorts Method](#) to set the port mapping for a Balanced - Balanced topology.

VB Syntax `var = balTopology.BB_BalPort2Negative`

Variable (Type) - Description

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

Return Type Long Integer

Default Not Applicable

Examples `variable = balTop.BB_BalPort2Negative 'Read`

C++ Syntax HRESULT get_BB_BalPort2Negative(long *bVal)

Interface IBalancedTopology

BB_BalPort2Positive Property

Description With a Balanced - Balanced topology, returns the PNA port number that is connected to the Positive side of the DUT's logical Port 2.

Use [SetBBPorts Method](#) to set the port mapping for a Balanced - Balanced topology.

VB Syntax `var = balTopology.BB_BalPort2Positive`

Variable (Type) - Description

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

Return Type Long Integer

Default Not Applicable

Examples `variable = balTop.BB_BalPort2Positive 'Read`

C++ Syntax HRESULT get_BB_BalPort2Positive(long *bVal)

Interface IBalancedTopology

BBalMeasurement Property

Description Sets and returns the measurement for the Balanced - Balanced topology.

VB Syntax *balMeas*.**BBalMeasurement** = *value*

Variable **(Type) - Description**

balMeas A BalancedMeasurement (**object**)

value **(String)** - Balanced - Balanced Measurement parameter. Not case sensitive. Choose from:

Sdd11	Sdd12	Sdc11	Sdc12
Sdd21	Sdd22	Sdc21	Sdc22
Scd11	Scd12	Sc11	Sc12
Scd21	Scd22	Sc21	Sc22
lmb1	lmb2	CMRR -(Sdd21/Sc11)	

Return Type String

Default Sdd11

Examples `balMeas.BBalMeasurement = "Sdd11" 'Write`
`variable = balMeas.BBalMeasurement 'Read`

C++ Syntax HRESULT get_BBalMeasurement(BSTR *pVal)
 HRESULT put_BBalMeasurement(BSTR newVal)

Interface IBalancedMeasurement

BeginResponse Property

Description When constructing a limit line, specifies the amplitude value of the start of a limit segment.

VB Syntax *limtseg*.BeginResponse = *value*

Variable (Type) - Description

limtseg A LimitSegment (**object**)

value (**double**) - Amplitude value. No units

Return Type Double

Default 0

Examples

```
Set limtseg = meas.LimitTest(1)
limtseg.BeginResponse = 10 'Write
```

```
BegResp = limtseg.BeginResponse 'Read
```

C++ Syntax HRESULT get_BeginResponse(double *pVal)
HRESULT put_BeginResponse(double newVal)

Interface ILimitSegment

BeginStimulus Property

Description When constructing a limit line, specifies the beginning X-axis value.

VB Syntax *limtseg.BeginStimulus* = *value*

Variable (Type) - Description

limtseg A LimitSegment (**object**)

value (**double**) - Stimulus value. No units

Return Type Double

Default 0

Examples

```
Set limtseg = meas.LimitTest(1)
limtseg.Type = naLimitSegmentType_Maximum
limtseg.BeginStimulus = 3e9
limtseg.EndStimulus = 4e9
limtseg.BeginResponse = 10
limtseg.EndResponse = 10
```

```
BegStim = limtseg.BeginStimulus 'Read
```

C++ Syntax HRESULT get_BeginStimulus(double *pVal)
HRESULT put_BeginStimulus(double newVal)

Interface ILimitSegment

Write/Read

BucketNumber Property

Description Sets or returns the bucket number (data point) for the active marker.**VB Syntax** *mark*.**BucketNumber** = *value***Variable (Type) - Description***mark* A Marker (**object**)*value* (**long integer**) - Data point. Choose any number between 0 and the measurement's number of data points - 1.

For example, with Number of points = 201, choose between 0 and 200

Return Type Long Integer**Default** The first marker is set to the middle of the span. Subsequent markers are set to the bucket number of the previously active marker.**Examples** `mark.BucketNumber = 100 'moves the active marker to data point 100 - Write``pointNumber = mark.BucketNumber 'returns the data point number the active marker is currently on. -Read`**C++ Syntax** HRESULT get_BucketNumber(long *pVal)
HRESULT put_BucketNumber(long newVal)**Interface** IMarker

Write/Read

C0 Property

Description Sets and Returns the C0 (C-zero) value (the first capacitance value) for the calibration standard.
To set the other capacitance values, use [C1](#), [C2](#), [C3](#)

VB Syntax `calstd.C0 = value`

Variable (Type) - Description

`calstd` A CalStandard (**object**). Use calKit.[GetCalStandard](#) to get a handle to the standard.

`value` (**single**) - Value for C0 in picofarads

Return Type Single

Default Not Applicable

Examples `calstd.C0 = 15 'Write the value of C0 to 15picofarads`

`cap0 = calstd.C0 'Read the value of C0`

C++ Syntax HRESULT get_C0(float *pVal)
HRESULT put_C0(float newVal)

Interface ICalStandard

C1 Property

Description Sets and Returns the C1 value (the second capacitance value) for the calibration standard.

To set the other capacitance values, use [C0](#), [C2](#), [C3](#)

VB Syntax `calstd.C1 = value`

Variable **(Type) - Description**

`calstd` A CalStandard **(object)**. Use `calKit.GetCalStandard` to get a handle to the standard.

`value` **(single)** - Value for C1 in picofarads

Return Type Single

Default Not Applicable

Examples `calstd.C1 = 15 'Write the value of C1 to 15picofarads`

`cap1 = calstd.C1 'Read the value of C1`

C++ Syntax HRESULT get_C1(float *pVal)
HRESULT put_C1(float newVal)

Interface ICalStandard

Write/Read

C2 Property

Description Sets and Returns the C2 value (the third capacitance value) for the calibration standard.
To set the other capacitance values, use C0, C1, C3

VB Syntax `calstd.C2 = value`

Variable (Type) - Description

`calstd` A CalStandard **(object)**. Use calKit.GetCalStandard to get a handle to the standard.

`value` **(single)** - Value for C2 in picofarads

Return Type Single

Default Not Applicable

Examples `calstd.C2 = 15 'Write the value of C2 to 15picofarads`

`cap2 = calstd.C2 'Read the value of C2`

C++ Syntax HRESULT get_C2(float *pVal)
HRESULT put_C2(float newVal)

Interface ICalStandard

Write/Read

C3 Property

Description Sets and Returns the C3 value (the fourth capacitance value) for the calibration standard.
To set the other capacitance values, use [C0](#), [C1](#), [C2](#)

VB Syntax `calstd.C3 = value`

Variable **(Type) - Description**

`calstd` A CalStandard **(object)**. Use calKit.[GetCalStandard](#) to get a handle to the standard.

`value` **(single)** - Value for C3 in picofarads

Return Type Single

Default Not Applicable

Examples `calstd.C3 = 15 'Write the value of C3 to 15picofarads`

`cap3 = calstd.C3 'Read the value of C3`

C++ Syntax HRESULT get_C3(float *pVal)
HRESULT put_C3(float newVal)

Interface ICalStandard

CalFactor Property

Description Sets or returns the cal factor value associated with a power sensor cal factor segment.

VB Syntax *calFactSeg*.**CalFactor** = *value*

Variable (Type) - Description

powerCalibrator **(object)** - A PowerSensorCalFactorSegment (object)

value **(double)** – Cal factor in percent. Choose any value between 1 and 150

Return Type Double

Default 0

Examples `calFactSeg.CalFactor = 98 'Write
factor = calFactSeg.CalFactor 'Read`

C++ Syntax HRESULT put_CalFactor(Double newVal);
HRESULT get_CalFactor(Double *pVal);

Interface IPowerSensorCalFactorSegment

CalibrationType Property

Description Specifies the type of calibration to perform or apply to the active measurement. This command will set the CalType for ports by inspecting the ports of the active measurement.

For example:

- If the measurement is an S23, it uses ports 2 and 3.
- If the measurement is an S22 it will use the legacy load port to figure out which two ports form the caltype. The legacy load port is set using [CreateMeasurement](#).
- If **naCalType_ThreePort_SOLT** is specified on a 4-port PNA, an E_NA_DEPRECATED_COMMAND error is returned. There is no way to determine the intended three ports.
- If **naCalType_FourPort_SOLT** is specified on a 4-port PNA, it is obvious that the ports involved are ports 1,2,3, and 4.

VB Syntax *meas*.**CalibrationType** = *type*

Variable **(Type) - Description**

meas A Measurement (**object**)

type (**enum NACalType**) - Calibration type. Choose from:

0 - naCalType_Response_Open

1 - naCalType_Response_Short

2 - naCalType_Response_Thru

3 - naCalType_Response_Thru_And_Isol

4 - naCalType_OnePort

5 - naCalType_TwoPort_SOLT

6 - naCalType_TwoPort_TRL

7 - naCalType_None

8 - naCalType_ThreePort_SOLT

9 - Custom

10 - naCalType_FourPort_SOLT

Return Type **NACalType**

Default naCalType_None

Examples `meas.CalibrationType = naCalType_Response_Open 'Write`

`meascal = meas.CalibrationType 'Read`

C++ Syntax HRESULT put_CalibrationType (tagNACalType CalType)
 HRESULT get_CalibrationType (tagNACalType* pCalType)

Interface IMeasurement

Read only

CalibrationName Property

Description Get the name of the current cal type.

VB Syntax *value* = *meas*.**CalibrationName**

Variable (Type) - Description

value **(string)** - Variable to store the returned value.

meas A Measurement **(object)**

Return Type String

Default Not Applicable

Examples `ct = meas.CalibrationName`

C++ Syntax HRESULT get_CalibrationName([out,retval] BSTR* CalibrationName);

Interface IMeasurement2

Read / Write

CalibrationPort Property

Description Specifies which SMC port to calibrate.

VB Syntax `SMC.CalibrationPort = value`

Variable (Type) - Description

`SMC` SMCType (object)

`value` (String) Port number to be calibrated. Choose from:

- **1** - SMC forward
- **2** - SMC reverse
- **Both**

Return Type String

Default 1

Examples `value = SMC.CalibrationPort = "Both"`

C++ Syntax `HRESULT put_CalibrationPort(BSTR port);`
`HRESULT get_CalibrationPort(BSTR *port);`

Interface SMCType
VMCType

CalibrationTypeID Property

Description Sets or returns the current cal type for custom measurements (FCA) using a Cal Type Name.

You can also use the CLSID or GUID associated with the cal type.

To select cal types for standard measurements, see [Calibration Type Property](#).

VB Syntax *meas*.**CalibrationTypeID** = *id*

Variable **(Type) - Description**

meas A Measurement **(object)**

id (String) Cal type identifier Name. Use one of the following:

Name - Choose one of the following:

- "VMC"
- "SMC_2P" or "SMC"
- "SMCRsp+IN"
- "SMCRsp+OUT"
- "SMCRsp"

You can also use a ClassID or GUID. The following are **examples**:

CLSID - "VectorMixerCal.VCMCType"

GUID - "{2061767B-0FE2-4F6F-86D0-9AB332B18DA5}"

Return Type String

Default Not Applicable

Examples

```
Dim pna
Dim m

Set pna = CreateObject("AgilentPNA835x.Application")
Set m = pna.ActiveMeasurement
m.CalibrationTypeID = "VMC"
m.ErrorCorrection = True
MsgBox m.CalibrationName
```

C++ Syntax HRESULT get_CalibrationTypeID([out, retval] BSTR* CalibrationTypeID);

HRESULT put_CalibrationTypeID([in] BSTR CalibrationTypeID);

Interface IMeasurement2

CalKitType Property

Description Sets and returns a calibration kit type for calibration or to be used for kit modification. To get a handle to this kit, use [app.ActiveCalKit](#).

There is also a [CalKitType](#) property on the GuidedCalibration object.

VB Syntax *object*.**CalKitType** = *value*

Variable (Type) - Description

object [calkit](#) (object) or
[Application](#) (object)

Note: **app**.CalKitType and **calkit**.calKitType perform exactly the same function.

value **(enum naCalKit)** - Calibration Kit type. Choose from:

1 - naCalKit_User1
2 - naCalKit_User2
3 - naCalKit_User3
4 - naCalKit_User4
..
..
..
49 - naCalKit_User49
50 - naCalKit_User50

These enumerated values correspond with the calibration kit ID on the [Advanced Cal Kit Modify dialog box](#).

To change the cal kit name, use [Name property](#).

Return Type NACalKit

Default Not Applicable

Examples `calkit.CalKitType = naCalKit_User27`

`kitype = app.CalKitType`

C++ Syntax HRESULT get_CalKitType(tagNACalKit *pVal);
HRESULT put_CalKitType(tagNACalKit newVal);

Interface IApplication
ICalKit

CalKitType Property

Description Sets and returns a calibration kit type for the specified port number to be used during the calibration.

Note: Sliding loads are not fully supported from the GuidedCalibration object. The **Measure** button must be pressed manually on the PNA.

VB Syntax *object.CalKitType (port) = value*

Variable **(Type) - Description**

object Any of the following:

[GuidedCalibration](#) (object)

[SMCType](#) (object)

[VMCType](#) (object)

port (Long) Port number the cal kit will be assigned to.

value **(string)** - Calibration Kit type.

Use [CompatibleCalKits](#) property for a list of valid Cal Kits.

Return Type String

Default Not Applicable

Examples `SMC.CalKitType(1) = naCalKit_User27`

`value = smc.CalKitType(1)`

C++ Syntax HRESULT get_CalKitType(long port, BSTR *calkit)
 HRESULT put_CalKitType(long port, BSTR calkit)

Interface IGuidedCalibration
 SMCType
 VMCType

Description Specifies the power level that is expected at the desired reference plane (DUT input or output). This is not used for segment sweep with independent power levels or power sweeps.

Note: Although this command still works, it is recommended that you specify cal power by setting the test port power and offset value.

VB Syntax *value* = *powerCalibrator*.**CalPower** (*chan*, *sourcePort*)

Variable (Type) - Description

value **(double)** - Variable to store the returned Cal power value in dBm.

powerCalibrator **(object)** - A SourcePowerCalibrator object

chan **(long integer)** - Channel number of the PNA.

sourcePort **(long integer)** - Source port number

Return Type None

Default 0

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.CalPower = -10 'Write
power = powerCalibrator.CalPower 'Read
```

C++ Syntax HRESULT get_CalPower(long channel, long sourcePort, double *pVal);

Interface ISourcePowerCalibrator

Center Property

Description Sets or returns the Center time of either Gating or Time Domain transform windows

VB Syntax *object.Center = value*

Variable **(Type) - Description**

object **(object)** As Gating
or
(object) As Transform

value **(double)** - Center time in seconds. Choose any number between:
 $\pm (\text{points}-1) / \text{frequency span}$

Return Type Double

Default 0

Examples

```
trans.Center = 4.5e-9 'sets the Center time of a transform
window -Write
gate.Center = 4.5e-9 'sets the Center time of a gating window -
Write
```

```
cnt = trans.Center 'Read
```

C++ Syntax HRESULT get_Center(double *pVal)
HRESULT put_Center(double newVal)

Interface ITransform
IGating

Read-only

Center Property

Description Returns the stimulus value of the center data point for the measurement. This function does NOT work for segment sweep measurements. To understand how this property is useful, see [IMeasurement2 Interface](#).

VB Syntax `value = meas.Center`

Variable **(Type) - Description**

`value` **(Double)** - Variable to store the returned value.

`meas` A Measurement **(object)**

Return Type Double

Default Not Applicable

Examples `Print meas.Center 'prints the center data point`

C++ Syntax `HRESULT get_Center(double * Val);`

Interface IMeasurement2

Write/Read

CenterFrequency Property

Description Sets or returns the center frequency of the channel
or
 Sets or returns the center frequency of the segment.
 see also Measurement2 interface

VB Syntax *object.CenterFrequency = value*

Variable (Type) - Description

object A Channel (**object**)
or
 A Segment (**object**)

value (**double**) - Center frequency in Hertz. Choose any number between the **minimum** and **maximum** frequencies of the analyzer.

Return Type Double

Default Center of the frequency range

Examples `chan.CenterFrequency = 4.5e9 'sets the center frequency of a linear sweep for the channel object -Write`

`centfreq = chan.CenterFrequency 'Read`

C++ Syntax HRESULT get_CenterFrequency(double *pVal)
 HRESULT put_CenterFrequency(double newVal)

Interface IChannel
 ISegment

Read-only

ChannelNumber Property

Description Returns the Channel number of the Channel or Measurement object.

VB Syntax *object*.ChannelNumber

Variable (Type) - Description

object A Channel (**object**)
or
A Measurement (**object**)

Return Type Long Integer

Default Not applicable

Examples

```
chanNum = chan.ChannelNumber 'returns the channel number
chanNum = meas.ChannelNumber 'returns the channel number of the
measurement
```

C++ Syntax HRESULT get_ChannelNumber(long *pVal)

Interface IChannel
IMeasurement

Read/Write

CharacterizeMixerOnly Property

Description Sets and returns whether to perform ONLY a mixer characterization.

VB Syntax `VMC.CharacterizeMixerOnly = bool`

Variable **(Type) - Description**

`VMC` VMCType (object)

`bool` (Boolean)

1 - Perform ONLY mixer characterization.

0 - Perform both mixer characterization and calibration.

Return Type Boolean

Default 0

Examples `value = VMC.CharacterizeMixerOnly`

C++ Syntax `HRESULT put_CharacterizeMixerOnly(VARIANT_BOOL
bCharMixerOnly);`

`HRESULT get_CharacterizeMixerOnly(VARIANT_BOOL
*bCharMixerOnly);`

Interface VMCType

Write/Read

CharFileName Property

Description Specifies the mixer characterization (.S2P) file and immediately loads the file. Also specify the use of a characterization file with [LoadCharFromFile Property](#)

VB Syntax `VMC.CharFileName = value`

Variable **(Type) - Description**

`VMC` [VMCType](#) (object)

`value` (String) Full path, file name, and extension of the mixer characterization file.

Return Type Not Applicable

Default Not Applicable

Examples `VMC.CharFileName = "C:\Program Files\Agilent\Network Analyzer\Documents\default.S2P"`

C++ Syntax `HRESULT put_CharFileName(BSTR filename);`
`HRESULT get_CharFileName(BSTR *filename);`

Interface `VMCType`

CharMixerReverse Property

Description	Specifies the direction in which to characterize the calibration mixer. Learn more about the calibration mixer.
VB Syntax	<code>VMC.CharMixerReverse = bool</code>
Variable	(Type) - Description
<code>VMC</code>	<code>VMCType</code> (object)
<code>bool</code>	(Boolean)
	0 - Characterize the calibration mixer in the SAME direction as that specified in the mixer setup.
	1 - Characterize the calibration mixer in the REVERSE direction as that specified in the mixer setup.
Return Type	Boolean
Default	0
Examples	<code>VMC.CharMixerReverse = 0</code>
C++ Syntax	<code>HRESULT put_CharMixerReverse(VARIANT_BOOL bcharReverse);</code> <code>HRESULT get_CharMixerReverse(VARIANT_BOOL *bcharReverse);</code>
Interface	VMCType2

Write/Read

CitiContents Property

Description Specifies the contents of subsequent citifile saves using `app.SaveCitiDataData` or `app.SaveCitiFormattedData`

VB Syntax `pref.CitiContents = value`

Variable (Type) - Description

pref A Preferences (**object**)

value (**string**) - Contents that will be saved with subsequent save commands. Choose from:

"**Single**" - Single trace

"**Displayed**" - All displayed traces

"**Auto**" - All displayed traces

Return Type String

Default "Auto"

Examples `pref.CitiContents = "Single" 'Write`

`content = pref.CitiContents 'Read`

C++ Syntax HRESULT get_CitiContents(BSTR *Contents)
HRESULT put_CitiContents(BSTR Contents)

Interface IPreferences

Write/Read

CitiFormat Property

Description	Specifies the format of subsequent citifile saves using <code>app.SaveCitiFormattedData</code>
VB Syntax	<code>pref.CitiFormat = value</code>
Variable	(Type) - Description
<i>pref</i>	A <u>Preferences</u> (object)
<i>value</i>	(string) - Format in which the citifile will be saved with subsequent save commands. Choose from: "MA" - Linear Magnitude / degrees "DB" - Log Mag / degrees "RI" - Real / Imaginary "Auto" - Format in which the trace is already displayed. If other than Log Mag, Linear Magnitude, or Real/Imag, then the format will be in Real/Imag.
Return Type	String
Default	"Auto"
Examples	<pre>pref.CitiFormat = "MA" 'Write format = pref.CitiFormat 'Read</pre>
C++ Syntax	HRESULT get_CitiFormat(BSTR *Format) HRESULT put_CitiFormat(BSTR Format)
Interface	IPreferences

CmnModeZConvPortImag Property

Description Sets the imaginary part of the impedance value for the common port impedance conversion function.

VB Syntax `fixture.CmnModeZConvPortImag(portNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`portNum` (**Integer**) Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` (**Double**) Imaginary part of the Impedance value. Choose a value between 0 and 1E18.

Return Type Double

Default 0

Examples `fixture.CmnModeZConvPortImag(2) = 75 'Write`

`value = fixture.CmnModeZConvPortImag(1) 'Read`

C++ Syntax HRESULT get_CmnModeZConvPortImag(short portNum, double *pVal)
 HRESULT put_CmnModeZConvPortImag(short portNum, double newVal)

Interface IFixturing2

CmnModeZConvPortReal Property

Description Sets the real part of the impedance value for the common port impedance conversion function.

VB Syntax `fixture.CmnModeZConvPortReal(portNum) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`portNum` **(Integer)** Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` **(Double)** Real part of the Impedance value. Choose a value between 0 and 1E18.

Return Type Double

Default See [Common Mode Port Z Conversion Default](#)

Examples `fixture.CmnModeZConvPortReal(2) = 75 'Write`

`value = fixture.CmnModeZConvPortReal(1) 'Read`

C++ Syntax HRESULT get_CmnModeZConvPortImag(short portNum, double *pVal)
HRESULT put_CmnModeZConvPortImag(short portNum, double newVal)

Interface IFixturing2

CmnModeZConvPortZ0 Property

Description Sets the impedance value for the common port impedance conversion function. Set either this single value or set the [real](#) and [imaginary](#) parts separately. The imaginary part is set to 0.0 using this command.

VB Syntax `fixture.CmnModeZConvPortZ0(portNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (object)

`portNum` (**Integer**) Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` (**Double**) Impedance value. Choose a value between 0 and 1E7.

Return Type Double

Default See [Common Mode Port Z Conversion Default](#)

Examples `fixture.CmnModeZConvPortZ0(2) = 75 'Write`

`value = fixture.CmnModeZConvPortZ0(1) 'Read`

C++ Syntax HRESULT get_CmnModeZConvPortImag(short portNum, double *pVal)
HRESULT put_CmnModeZConvPortImag(short portNum, double newVal)

Interface IFixturing2

CmnModeZConvState Property

Description Turns ON or OFF 4-port common port impedance conversion function. Must also set the fixture simulator function to ON using [FixturingState Property](#).

VB Syntax `fixture.CmnModeZConvState = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`value` (**Boolean**)

False - Turns common port impedance conversion OFF

True - Turns common port impedance conversion ON

Return Type Boolean

Default False (OFF)

Examples `fixture.CmnModeZConvState = 0 'Write`

`value = fixture.CmnModeZConvState 'Read`

C++ Syntax HRESULT get_CmnModeZConvState(VARIANT_BOOL *pVal)
HRESULT put_CmnModeZConvState(VARIANT_BOOL newVal)

Interface IFixturing2

Read-only

CompatibleCalKits Property

Description Returns a list of cal kits that are compatible with the connector type for the specified port.

VB Syntax *value* = *obj*.CompatibleCalKits (*port*)

Variable **(Type) - Description**

value (Variant) Variable to store the returned list of CalKits.

obj Any of the following:

GuidedCalibration (object)

SMCType (object)

VMCType (object)

port (Long) Port number for which you want compatible kits.

Return Type Variant

Default Not Applicable

Examples

```
Dim kits As Variant
kits = MySMC.CompatibleCalKits(1)
```

C++ Syntax HRESULT get_CompatibleCalKits(long port, VARIANT* Kits);

Interface IGuidedCalibration

SMCType

VMCType

ConnectorType Property

Description Sets or queries the connector type for the specified port.

VB Syntax *obj.ConnectorType (port) = value*

Variable (Type) - Description

obj Any of the following:

GuidedCalibration (object)

SMCType (object)

VMCType (object)

port (Long) Port number of the connector type

value (String) - Connector type.

Use ValidConnectorType Property to list connector types.

Return Type String

Default None

Examples

```
Dim value As String
Value = MySMC.ConnectorType
```

C++ Syntax HRESULT get_ConnectorType(long port, BSTR *connector)

HRESULT put_ConnectorType(long port, BSTR connector)

Interface IGuidedCalibration

SMCType

VMCType

ControlLines Property

Description Sets the control lines of the specified E5091A. Control lines, provided through a E5091A front panel connector, are used to control external equipment such as a part handler. See your E5091A documentation to learn more about control lines.

VB Syntax `testsets(1).ControlLines (chNum) = value`

Variable (Type) - Description

`testsets(1)` An item from Testsets (**collection**)
Learn how to identify a testset in the collection.

`chNum` (**Integer**) Channel number of the measurement.

`value` (**Double**) Data value used to set control lines. Values are obtained by adding weights from the following table that correspond to individual lines. HIGH =1; LOW=0.

Line	Weight
1	1
2	2
3	4
4	8
5	16
6	32
7	64
8	128

0 - Sets all lines low

255 - Sets all lines high

Return Type Variant

Default 0

Examples `'The following sets line 3 and 4 high; all other lines low.`

```
testset1.ControlLines(2) = 12
```

[See Example Program](#)

C++ Syntax `HRESULT get_ControlLines(long channelNum, VARIANT *stateByte);`
`HRESULT put_ControlLines(long channelNum, VARIANT stateByte);`

Interface IE5091Testsets

Read-only

Count Property

Description Returns the number of items in a collection of objects.

VB Syntax *object*.Count

Variable (Type) - Description

object Any of the following **(objects)**:
Cal Sets collection
CalFactorSegments collection
Channels collection
LimitTest collection
Measurements collection
NAWindows collection
PowerLossSegments collection
PowerSensors collection
Segments collection
Traces collection

Return Type Long Integer

Default Not applicable

Examples `numofchans = chans.Count 'return the number of channels
-Read`

C++ Syntax HRESULT get_Count(long *p<interface>)

Interface ICal Sets
ICalFactorSegments
IChannels
ILimitTest
IMeasurements
INAWindows
IPowerLossSegments
IPowerSensors
ISegments
ITraces

CouplePorts Property

Description Turns ON and OFF port power coupling. ON means the power level is the same for both ports. OFF means the power level may be set independently for each port.

VB Syntax `object.CouplePorts = value`

Variable (Type) - Description

object Channel (**object**)
or
 CalSet (**object**) - Read-only property

value (**enum NAStates**) Choose from:
0 - NaOff - Turns coupling OFF
1 - NaOn - Turns coupling ON

Return Type Long Integer
1 - ON
0 - OFF

Default NaON (1)

Examples `chan.CouplePorts = NaOff 'Write`

`couplport = chan.CouplePorts 'Read`

C++ Syntax HRESULT get_CouplePorts(tagNAStates *pState)
 HRESULT put_CouplePorts(tagNAStates newState)

Interface IChannel
 |CalSet3

CoupleChannelParams Property

Description Turns ON and OFF Time Domain Trace Coupling. All of the measurements in the specified channel are coupled.

- To select Transform parameters to couple, use [Trans.CoupledParameters Property](#)
- To select Gating parameters to couple, use [Gate.CoupledParameters Property](#)

VB Syntax `chan.CoupleChannelParams = state`

Variable **(Type) - Description**

chan A [Channel](#) (**object**)

state (**boolean**)
0 - Turns Trace Coupling OFF
1 - Turns Trace Coupling ON

Return Type Boolean

Default 1 - ON

Examples `chan.CoupleChannelParams = 1 'Write`

`couple = chan.CoupleChannelParams 'Read`

C++ Syntax HRESULT get_CoupleChannelParams(VARIANT_BOOL *isCoupled);
 HRESULT put_CoupleChannelParams(VARIANT_BOOL isCoupled);

Interface IChannel5

CoupledMarkers Property

Description Sets and Reads the state of Coupled Markers (ON and OFF)

VB Syntax `app.CoupledMarkers = state`

Variable (Type) - Description

`app` An Application (**object**)

`state` (**boolean**)
False (0) - Turns Coupled Markers OFF
True (1) - Turns Coupled Markers ON

Return Type Boolean
0 - OFF
1 - ON

Default OFF (0)

Examples `app.CoupledMarkers = True 'Write`

`coupl = app.CoupledMarkers 'Read`

C++ Syntax HRESULT put_CoupledMarkers(VARIANT_BOOL bState)
HRESULT get_CoupledMarkers(VARIANT_BOOL *bState)

Interface IApplication

CoupledParameters Property (Gating)

Description Specifies the time domain gating parameters to be coupled. The settings for those parameters will be copied from the active measurement to all other measurements on the channel.

To turn coupling ON and OFF, use CoupleChannelParams Property

To specify Transform parameters to couple, use Transform.CoupledParameters Property

VB Syntax `gate.CoupledParameters = value`

Variable (Type) - Description

trans A Gating (object)

value **(Enum As NAGatingCoupledParams)** - Parameters to couple. To specify more than one parameter, add the numbers. Choose from:

1 - naGatingStimulusCoupled (Start, Stop, Center, and Span TIME settings.)

2 - naGateStateCoupled (ON / OFF)

4 - naGatingShapeCoupled (Minimum, Normal, Wide, and Maximum)

8 - naGatingTypeCoupled (Bandpass and Notch)

Return Type Enum

Default 29

Examples `gate.CoupledParameters = 15 'Couple all parameters`

`CP = gate.CoupledParameters 'Read`

C++ Syntax HRESULT get_CoupledParameters(long *IParams);

HRESULT put_CoupledParameters(long IParams);

Interface IGating2

CoupledParameters Property (Transform)

Description Specifies the time domain transform parameters to be coupled. The settings for those parameters will be copied from the active measurement to all other measurements on the channel.

To turn coupling ON and OFF, use [CoupleChannelParams Property](#)

To specify Gating parameters to couple, use [Gate.CoupledParameters Property](#)

VB Syntax *trans.CoupledParameters* = *value*

Variable (Type) - Description

trans A [Transform](#) (object)

value **(Enum As NATransformCoupledParams)** - Parameters to couple. To specify more than one parameter, add the numbers. Choose from:

1 - naTransformStimulusCoupled (Start, Stop, Center, and Span TIME settings.)

2 - naTransformStateCoupled (ON / OFF)

4 - naTransformWindowCoupled (Kaiser Beta / Impulse Width)

8 - naTransformModeCoupled (Low Pass Impulse, Low Pass Step, Band Pass)

16 - naTransformDistMkrUnitCoupled (Distance maker Units)

Return Type Enum

Default 29

Examples `trans.CoupledParameters = 31 'Couple all parameters`

`CP = trans.CoupledParameters 'Read`

C++ Syntax HRESULT get_CoupledParameters(long *IParams);
HRESULT put_CoupledParameters(long IParams);

Interface ITransform2

Write/Read

CW Frequency Property

Description Set the Continuous Wave (CW) frequency. Must first send `chan.SweepType = naCWTimeSweep`**VB Syntax** `object.CWFrequency = value`**Variable** **(Type) - Description***object* Channel **(object)****or**CalSet **(object)** - Read-only property*value* **(double)** CW frequency. Choose any number between:
the **minimum** and **maximum** frequency limits of the analyzer
Units are Hz**Return Type** Double**Default** 1e9**Examples** `chan.CWFrequency = 5e9 'Write``cfreq = chan.CWFrequency 'Read`**C++ Syntax** HRESULT put_CWFrequency(double newVal)
HRESULT get_CWFrequency(double *pVal)**Interface** IChannel
|CalSet3

Write/Read

Delay Property

Description Sets and Returns the electrical delay value for the calibration standard.

VB Syntax `calstd.Delay = value`

Variable **(Type) - Description**

calstd A CalStandard **(object)**. Use `calKit.GetCalStandard` to get a handle to the standard.

value **(single)** - Electrical delay in seconds

Return Type Single

Default Not Applicable

Exaamples `calstd.Delay = .00015 'Write the Delay .00015 seconds`

`stdDelay = calstd.Delay 'Read the value of Delay`

C++ Syntax HRESULT get_Delay(float *pVal)
HRESULT put_Delay(float newVal)

Interface ICalStandard

DeltaMarker Property

Description Sets a marker as a delta marker. The reference marker must already be turned ON. See [meas.ReferenceMarkerState](#)

VB Syntax `mark.DeltaMarker = state`

Variable **(Type) - Description**

app A Marker **(object)**

state **(boolean)** -
ON (1) marker is a delta marker
OFF (0) marker is NOT a delta marker

Return Type Boolean

Default OFF (0)

Examples `mark.DeltaMarker = True 'Write`

`delta = mark.DeltaMarker 'Read`

C++ Syntax HRESULT get_DeltaMarker(VARIANT_BOOL bState)
HRESULT put_DeltaMarker(VARIANT_BOOL *bState)

Interface IMarker

Description Property

Description Sets or returns the descriptive string assigned to the Cal Set. Change this string so that you can easily identify each Cal Set constructed.

VB Syntax *CalSet.Description* = *value*

Variable (Type) - Description

CalSet **(object)** - A Cal Set object

value **(string)** – Description of the Cal Set

Return Type String

Default "CalSet_n" where n is an integer number.

Examples

```
CalSet.Description = "My Cal Set" 'Write
desc = CalSet.Description 'Read
```

C++ Syntax HRESULT get_Description(BSTR *pVal)
HRESULT put_Description(BSTR newVal);

Interface ICalSet

DiffPortMatch_C Property

Description Sets the Capacitance value of the differential matching circuit.

VB Syntax `fixture.DiffPortMatch_C (portNum) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`portNum` **(Integer)** Balanced (logical) port number. Choose from logical ports 1,2 ,3. [Learn more about logical ports.](#)

`value` **(Double)** Capacitance value in farads. Choose a value between **-1E18** to **1E18**.

Return Type Double

Default 0

Examples `fixture.DiffPortMatch_C(2) = 1e-6 'Write`

`value = fixture.DiffPortMatch_C(1) 'Read`

C++ Syntax HRESULT get_DiffPortMatch_C(short portNum, double *pVal)
HRESULT put_DiffPortMatch_C(short portNum, double newVal)

Interface IFixturing2

DiffPortMatch_G Property

Description Sets the Conductance value of the differential matching circuit.

VB Syntax `fixture.DiffPortMatch_G(portNum) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`portNum` **(Integer)** Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` **(Double)** Conductance value in siemens. Choose a value between **-1E18** to **1E18**.

Return Type Double

Default 0

Examples `fixture.DiffPortMatch_G(2) = 1e-3 'Write`

`value = fixture.DiffPortMatch_G(1) 'Read`

C++ Syntax HRESULT get_DiffPortMatch_G(short portNum, double *pVal)
HRESULT put_DiffPortMatch_G(short portNum, double newVal)

Interface IFixturing2

DiffPortMatch_L Property

Description Sets the Inductance value of the differential matching circuit.

VB Syntax `fixture.DiffPortMatch_L(portNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`portNum` (**Integer**) Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` (**Double**) Inductance value in henries. Choose a value between **-1E18** to **1E18**.

Return Type Double

Default 0

Examples `fixture.DiffPortMatch_L(2) = 1e-3 'Write`

```
value = fixture.DiffPortMatch_L(1) 'Read
```

C++ Syntax HRESULT get_DiffPortMatch_L(short portNum, double *pVal)
HRESULT put_DiffPortMatch_L(short portNum, double newVal)

Interface IFixturing2

DiffPortMatch_R Property

Description Sets the Resistance value of the differential matching circuit.

VB Syntax `fixture.DiffPortMatch_R(portNum) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`portNum` **(Integer)** Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` **(Double)** Resistance value in ohms. Choose a value between **-1E18** to **1E18**.

Return Type Double

Default 0

Examples `fixture.DiffPortMatch_R(2) = 1e3 'Write`

```
value = fixture.DiffPortMatch_R(1) 'Read
```

C++ Syntax HRESULT get_DiffPortMatch_R(short portNum, double *pVal)
HRESULT put_DiffPortMatch_R(short portNum, double newVal)

Interface IFixturing2

DiffPortMatchMode Property

Description Sets the differential matching circuit type. To select a user-defined circuit, specify IN ADVANCE the 2-port touchstone filename with [DiffPortMatch_UserFilename Property](#). If you do not specify the appropriate file and you select USER, an error occurs and naNO_CIRCUIT is automatically selected.

VB Syntax `fixture.DiffPortMatchMode(pNum) = value`

Variable (Type) - Description

fixture A [Fixturing](#) (object)

pNum (**Integer**) Balanced (logical) port number. Choose from logical ports **1, 2, or 3**. [Learn more about logical ports.](#)

value (**Enum as NADiffPortMatchCircuitMode**) Choose from:
0 or **naSHUNT_L_SHUNT_C_CIRCUIT** - Specifies the circuit that consists of shunt L and shunt C.
1 or **naUSER_FILE_CIRCUIT** - Specifies the user-defined circuit.
2 or **naNO_CIRCUIT** - Specifies no-circuit.

Return Type Enum

Default **naSHUNT_L_SHUNT_C_CIRCUIT**

Examples `fixture.DiffPortMatchMode(2) = naNO_CIRCUIT 'Write`

`value = fixture.DiffPortMatchMode(1) 'Read`

C++ Syntax HRESULT get_DiffPortMatchMode(short port, tagNADiffPortMatchCircuitMode *eVal)
 HRESULT put_DiffPortMatchMode(short port, tagNADiffPortMatchCircuitMode eVal)

Interface IFixturing2

DiffPortMatchState Property

Description Turns ON or OFF 4-port differential port matching function. Must also set the fixture simulator function to ON using [FixturingState Property](#).

VB Syntax `fixture.DiffPortMatchState = value`

Variable **(Type) - Description**

fixture A [Fixturing](#) (**object**)

value (**Boolean**)

False - Turns differential port matching OFF

True - Turns differential port matching ON

Return Type Boolean

Default False (OFF)

Examples `fixture.DiffPortMatchState = 0 'Write`

`value = fixture.DiffPortMatchState 'Read`

C++ Syntax HRESULT get_DiffPortMatchState(VARIANT_BOOL *pVal)
HRESULT put_DiffPortMatchState(VARIANT_BOOL newVal)

Interface IFixturing2

DiffPortMatchUserFilename Property

Description Specifies the 2-port touchstone file in which the information on the user-defined differential matching circuit is saved. Following this command, send [DiffPortMatchCircuit Property](#). If the specified file does not exist, an error occurs when you set the type of differential matching circuit to USER.

VB Syntax `fixture.DiffPortMatchUserFilename(pNum) = value`

Variable (Type) - Description

fixture A [Fixturing](#) (object)

pNum (**Integer**) Balanced (logical) port number. Choose from logical ports **1**, **2** or **3**. [Learn more about logical ports.](#)

value (**String**) Full path, file name, and extension (.s2P) of the de-embedding circuit. Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents

Return Type String

Default Not Applicable

Examples

```
fixture.DiffPortMatchUserFilename(2) = "C:\Program Files\Agilent\Network Analyzer\Documents\myFile.s4p" 'Write
value = fixture.DiffPortMatchUserFilename(1) 'Read
```

C++ Syntax HRESULT get_DiffPortMatchUserFilename(short port, BSTR *bstrFile)
 HRESULT put_DiffPortMatchUserFilename(short port, BSTR bstrFile)

Interface IFixturing2

DiffZConvPortImag Property

Description Sets the imaginary part of the impedance value for the differential port impedance conversion function.

VB Syntax `fixture.DiffZConvPortImag(portNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`portNum` (**Integer**) Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` (**Double**) Imaginary part of the Impedance value. Choose a value between 0 and 1E18

Return Type Double

Default 0

Examples `fixture.DiffZConvPortImag(2) = 75 'Write`

`value = fixture.DiffZConvPortImag(1) 'Read`

C++ Syntax HRESULT get_DiffZConvPortImag(short portNum, double *pVal)
HRESULT put_DiffZConvPortImag(short portNum, double newVal)

Interface IFixturing2

DiffZConvPortReal Property

Description Sets the imaginary part of the impedance value for the differential port impedance conversion function.

VB Syntax `fixture.DiffZConvPortReal(portNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`portNum` (**Integer**) Balanced (logical) port number. Choose from logical ports 1, 2, or 3. [Learn more about logical ports.](#)

`value` (**Double**) Real part of the Impedance value. Choose a value between 0 and 1E18

Return Type Double

Default See [Differential Port Z Conversion Default](#)

Examples `fixture.DiffZConvPortReal(2) = 75 'Write`

```
value = fixture.DiffZConvPortReal(1) 'Read
```

C++ Syntax HRESULT get_DiffZConvPortReal(short portNum, double *pVal)
HRESULT put_DiffZConvPortReal(short portNum, double newVal)

Interface IFixturing2

DiffZConvPortZ0 Property

Description Sets the impedance value for the differential port impedance conversion function. Set either this single value or set the real and imaginary parts separately. The imaginary part is set to 0.0 using this command.

VB Syntax `fixture.DiffZConvPortZ0(portNum) = value`

Variable (Type) - Description

`fixture` A Fixturing (**object**)

`portNum` (**Integer**) Balanced (logical) port number. Choose from logical ports 1, 2, or 3. Learn more about logical ports.

`value` (**Double**) Impedance value. Choose a value between 0 and 1E18

Return Type Double

Default See Differential Port Z Conversion Default

Examples `fixture.DiffZConvPortZ0(2) = 75 'Write`

`value = fixture.DiffZConvPortZ0(1) 'Read`

C++ Syntax HRESULT get_DiffZConvPortZ0(short portNum, double *pVal)
 HRESULT put_DiffZConvPortZ0(short portNum, double newVal)

Interface IFixturing2

DiffZConvState Property

Description Turns ON or OFF 4-port differential impedance conversion function. Must also set the fixture simulator function to ON using [FixturingState Property](#).

VB Syntax `fixture.DiffZConvState = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`value` (**Boolean**)

False - Turns differential impedance conversion OFF.

True - Turns differential impedance conversion ON.

Return Type Boolean

Default False (OFF)

Examples `fixture.DiffZConvState = 0 'Write`

`value = fixture.DiffZConvState 'Read`

C++ Syntax HRESULT get_DiffZConvState(VARIANT_BOOL *pVal)
HRESULT put_DiffZConvState(VARIANT_BOOL newVal)

Interface IFixturing2

Write/Read

Format Property

Description Sets or returns the display format of the measurement.**VB Syntax** `meas.Format = value`**Variable** **(Type) - Description***meas* A Measurement (**object**)*value* (**enum NADataFormat**) - Choose from:

0 - naDataFormat_LinMag

1 - naDataFormat_LogMag

2 - naDataFormat_Phase

3 - naDataFormat_Polar

4 - naDataFormat_Smith

5 - naDataFormat_Delay

6 - naDataFormat_Real

7 - naDataFormat_Imaginary

8 - naDataFormat_SWR

Return Type Long Integer**Default** 1 - naDataFormat_LogMag**Examples** `meas.Format = naDataFormat_Real 'Write``fmt = meas.Format 'Read`**C++ Syntax** HRESULT get_Format(tagDataFormat *pVal)
HRESULT put_Format(tagDataFormat newVal)**Interface** IMeasurement

Write-Read

DisplayAutomationErrors Property

Description Enables or disables automation error messages from being displayed on the screen.

VB Syntax `app.DisplayAutomationErrors = value`

Variable **(Type) - Description**

app An Application (**object**)

value (Boolean)

True allows error to show on display,

False turns error off from display.

Return Type Boolean

Default True

Examples

```
Dim app As Application
Set app = New Application
app.DisplayAutomationErrors = False      'Turns off display
print app.DisplayAutomationErrors      'prints False
```

C++ Syntax HRESULT get_DisplayAutomationErrors(VARIANT_BOOL * Val);
HRESULT put_DisplayAutomationErrors(VARIANT_BOOL Val);

Interface IApplication2

DisplayGlobalPassFail Property

Description Shows or hides the dialog which displays global pass/fail results. [Learn more about Global Pass/Fail.](#)

VB Syntax `app.DisplayGlobalPassFail = value`

Variable **(Type) - Description**

app An [Application](#) (**object**)

value (Boolean)

True (1) - displays the pass/fail dialog.

False(0) - hides the pass/fail dialog.

Return Type Boolean

Default False

Examples

```
Dim app As Application
Set app = New Application
app.DisplayGlobalPassFail = true 'shows dialog
```

C++ Syntax HRESULT get_DisplayGlobalPassFail(VARIANT_BOOL * Val);
HRESULT put_DisplayGlobalPassFail(VARIANT_BOOL Val);

Interface IApplication6

Distance Property

Description Set or query marker distance on a time domain trace.

The Write command moves the marker to the specified distance value. Once moved, you can read the Y axis value or read the X-axis time value. (Distance is calculated from the X-axis time value.)

The Read command reads the distance of the marker.

If the marker is set as delta, the WRITE and READ data is relative to the reference marker.

VB Syntax `mark.Distance = value`

Variable (Type) - Description

`mark` A Marker (object)

`value` (**double**) - Marker distance in the unit of measure specified with DistanceMarkerUnit Property

Return Type Double

Default Not Applicable

Examples `mark.Distance = 3e9 'Write`

`XVal = mark.Distance 'Read`

C++ Syntax HRESULT get_Distance(double *pVal);
HRESULT put_Distance(double newVal);

Interface IMarker2

Write/Read

DistanceMarkerMode Property

Description Specifies the measurement type in order to determine the correct marker distance.

- Select Auto for S-Parameter measurements.
- Select Reflection or Transmission for arbitrary ratio or unratioed measurements.

This settings affects the display of ALL markers for only the ACTIVE measurement.

VB Syntax *trans.DistanceMarkerMode = value*

Variable **(Type) - Description**

trans A Transform (**object**)

value **(enum As NADistanceMarkerMode)** - Choose from:

- 0 - naDistanceMarkerModeAuto
- 1 - naDistanceMarkerModeReflection
- 2 - naDistanceMarkerModeTransmission

Return Type Enum

Default 0 - naDistanceMarkerModeAuto

Examples `trans.DistanceMarkerMode = naDistanceMarkerModeReflection 'Write`
`DMM = trans.DistanceMarkerMode 'Read`

C++ Syntax HRESULT get_DistanceMarkerMode(tagNADistanceMarkerMode *pVal);
 HRESULT put_DistanceMarkerMode(tagNADistanceMarkerMode newVal);

Interface ITransform2

Write/Read

DistanceMarkerUnit Property

Description Specifies the unit of measure for the display of marker distance values. This settings affects the display of ALL markers for only the ACTIVE measurement (unless Distance Marker Units are coupled using [CoupledParameters Property](#)).

VB Syntax *trans.DistanceMarkerUnit* = *value*

Variable (Type) - Description

trans A [Transform](#) (object)

value **(Enum As NADistanceMarkerUnit)** - Distance Marker Units. Choose from

0 - naDistanceMarkerUnitMeter

1 - naDistanceMarkerUnitFeet

2 - naDistanceMarkerUnitInch

Return Type Enum

Default 0 - naDistanceMarkerUnitMeter

Examples `trans.DistanceMarkerUnit = naDistanceMarkerUnitFeet 'sets the`

`U = trans.DistanceMarkerUnit 'Read`

C++ Syntax HRESULT get_DistanceMarkerUnit(tagNADistanceMarkerUnit *pVal);
 HRESULT put_DistanceMarkerUnit(tagNADistanceMarkerUnit newVal);

Interface ITransform2

Do1PortEcal Property

Description	Specify ECAL or Mechanical calibration for the mixer characterization portion of a VMC calibration.
VB Syntax	<code>VMC.Do1PortEcal = bool</code>
Variable	(Type) - Description
<code>VMC</code>	<u>VMCType</u> (object)
<code>bool</code>	(Boolean)
	1 - ECAL
	0 - Mechanical
Return Type	Boolean
Default	0
Examples	<code>value = VMC.Do1PortEcal</code>
C++ Syntax	<code>HRESULT put_Do1PortEcal(VARIANT_BOOL bDoEcal);</code> <code>HRESULT get_Do1PortEcal(VARIANT_BOOL *bDoEcal);</code>
Interface	VMCType

Do2PortEcal Property

Description Specify ECAL or Mechanical calibration. For VMC, this selection only applies to the 2-port calibration portion. For mixer characterization (VMC), use [Do1PortEcal Property](#)

VB Syntax *object.Do2PortEcal = bool*

Variable **(Type) - Description**

object [SMCType](#) (object) or
[VMCType](#) (object)

bool (Boolean)
1 - ECAL
0 - Mechanical

Return Type Boolean

Default 0

Examples `value = VMC.Do2PortEcal`

C++ Syntax HRESULT put_Do2PortEcal(VARIANT_BOOL bDoEcal);
HRESULT get_Do2PortEcal(VARIANT_BOOL *bDoEcal);

Interface SMCType
VMCType

Read-only

Domain Property

Description Returns the domain (frequency,time, power) of the measurement. To understand how this property is useful, see [IMeasurement2 Interface](#).

VB Syntax `value = meas.Domain`

Variable **(Type) - Description**

value **(Enum** as NADomainType) - variable to store the returned value

0 - Frequency

1 - Time

2 - Power

meas A Measurement **(object)**

Return Type Enum as NADomainType

Default Not Applicable

Examples `Print meas.Domain 'prints the value of the domain enum`

C++ Syntax `HRESULT get_Domain(tagNADomainType * Val);`

Interface IMeasurement2

DUTTopology Property

Description Returns the device topology setting.

VB Syntax `balTopology.DUTTopology = value`

Variable **(Type) - Description**

balTopology A BalancedTopology (**object**)

value **(enum NADUTTopology) - Choose either:**

0 naSEBal: Single-Ended - Balanced measurement

1 naSESEBal: Single-Ended - Single-Ended - Balanced measurement

2 naBalBal: Balanced - Balanced measurement

Return Type Enum as NADUTTopology

Default naSEBal

Examples `balTop.DUTTopology = naSESEBal 'Write`

`DutTop = balTop.DUTTopology 'Read`

C++ Syntax HRESULT get_DUTTopology(tagNADUTTopology* pVal)
 HRESULT put_DUTTopology(tagNADUTTopology newVal)

Interface IBalancedTopology

Write/Read

DwellTime Property

Description Sets or returns the dwell time at the start of each sweep point for all measurements in a channel. Dwell time is only available with Chan.SweepGenerationMode = **naSteppedSweep** (not naAnalogSweep).

Sets or returns the dwell time of a specified sweep segment.

VB Syntax *object.DwellTime* = *value*

Variable (Type) - Description

object A Channel (object)
 or CalSet (object) - Read-only property
 or Segment (object)

value **(double)** - Dwell Time in seconds. Choose any number between **0** and **86400**

Return Type Double

Default 0

Examples `chan.DwellTime = 3e-3 'sets the dwell time for the channel -Write`

`segs(3).DwellTime = 1e9 'sets the dwell time of segment 3 -Write`

`dwell = chan.DwellTime 'Read`

C++ Syntax HRESULT get_DwellTime(double *pVal)
 HRESULT put_DwellTime(double newVal)

Interface IChannel
 ISegment
 ICalSet3

ECALCharacterization Property

Description	Specifies the characterization data within an ECal module to be used for the SMC calibration. Learn more about ECal User Characterization .
VB Syntax	<code>SMC.ECALCharacterization(mod) = value</code>
Variable	(Type) - Description
<code>SMC</code>	<code>SMCType</code> (object)
<code>module</code>	1- ECal module
<code>value</code>	(Long) – Characterization data within the ECal module to be used for ECal operations. Choose from: 0 – Factory Characterization 1 – UserCharacterization1 2 – UserCharacterization2 3 – UserCharacterization3 4 – UserCharacterization4 5 – UserCharacterization5
Return Type	Long
Default	0 - Factory Characterization
Examples	<code>SMC.ECALCharacterization(1) = 2</code>
C++ Syntax	HRESULT put_ECALCharacterization(long moduleNumber, long characterization); HRESULT get_ECALCharacterization(long moduleNumber, long* characterization);
Interface	ICalibrator2

ECALCharacterization Property

Description	Specifies the characterization data within an ECal module to be used, and the portion of the VMC calibration. Learn more about ECal User Characterization .
VB Syntax	<code>VMC.ECALCharacterization (module,port) = value</code>
Variable	(Type) - Description
<code>VMC</code>	<code>VMCType</code> (object)
<code>module</code>	(long integer) 1 - ECAL module
<code>port</code>	(boolean) True - 2-port calibration portion of the VMC False - 1-port (mixer characterization portion of the VMC cal
<code>value</code>	(Long) – Characterization data within the ECal module to be used for ECal operations. Choose from: 0 – Factory Characterization 1 – UserCharacterization1 2 – UserCharacterization2 3 – UserCharacterization3 4 – UserCharacterization4 5 – UserCharacterization5
Return Type	Long
Default	0 - Factory Characterization
Examples	<code>VMC.ECALCharacterization (1,True) = 4</code>
C++ Syntax	HRESULT put_ECALCharacterization(long moduleNumber, long characterization); HRESULT get_ECALCharacterization(long moduleNumber, long* characterization);
Interface	ICalibrator2

ECALCharacterizationEx Property

Description	This property replaces ECALCharacterization Property . Specifies the characterization data within an ECal module to be used for the calibration. Learn more about ECal User Characterization .
VB Syntax	<i>cal</i> . ECALCharacterizationEx (<i>module</i>) = <i>value</i>
Variable	(Type) - Description
<i>cal</i>	Calibrator (object)
<i>module</i>	(long integer) Optional argument. ECal module. Choose from modules 1 through 8 Use IsECALModuleFoundEx to determine the number of modules connected to the PNA Use GetECALModuleInfoEx to returns the model and serial number of each module.
<i>value</i>	(Long) – Characterization data within the ECal module to be used for ECal operations. Choose from: 0 – Factory Characterization 1 – UserCharacterization1 2 – UserCharacterization2 3 – UserCharacterization3 4 – UserCharacterization4 5 – UserCharacterization5
Return Type	Long
Default	0 - Factory Characterization
Examples	<code>cal.ECALCharacterizationEx (4) = 2</code>
C++ Syntax	HRESULT put_ECALCharacterizationEx(long moduleNumber, long characterization); HRESULT get_ECALCharacterizationEx(long moduleNumber, long* characterization);
Interface	ICalibrator4

ECALIsolation Property **OBSOLETE**

Description	<p>Note: The PNA no longer allows ECAL isolation to be performed. The inherent isolation of the PNA is better than that attained with correction using an ECAL module.</p> <p>Specifies whether the acquisition of the ECAL calibration should include isolation or not.</p>
VB Syntax	<code>cal.ECALIsolation = value</code>
Variable	(Type) - Description
<i>cal</i>	A Calibrator (object)
<i>value</i>	(boolean)
	False (0) - Exclude Isolation
	True (1) - Include Isolation
Return Type	Boolean
Default	False (0)
Examples	<pre>Dim oPNA as AgilentPNA835x.Application Dim oCal as Calibrator Set oPNA = CreateObject("AgilentPNA835x.Application", "MachineName") Set oCal = oPNA.ActiveChannel.Calibrator ' Uncomment the following line to have the cal include isolation ' oCal.ECALIsolation = True ' Uncomment the following line to have the cal omit isolation 'oCal.ECALIsolation = False oCal.DoECAL2Port ' Do the cal</pre>
C++ Syntax	<pre>HRESULT put_ECALIsolation (VARIANT_BOOL bIsolationState); HRESULT get_ECALIsolation (VARIANT_BOOL *bIsolationState);</pre>
Interface	Calibrator

EcalOrientation Property

Description Specifies which port of the ECal module is connected to which port of the PNA when the AutoOrient property = False.

VB Syntax `SMC.EcalOrientation (mod) = value`

Variable **(Type) - Description**

SMC SMCType (object)

mod (Long)
1 - Use ECAL Module for the calibration.

value **(string)** -Format this parameter in the following manner:
Aw,Bx,Cy,Dz
where

- A, B, C, and D are literal ports on the ECAL module
- w,x,y, and z are substituted for PNA port numbers to which the ECAL module port is connected.

Ports of the module which are not used are omitted from the string.

For example, on a 4-port ECal module with

- port A connected to PNA port 2
- port B connected to PNA port 3
- port C not connected
- port D connected to PNA port 1

the string would be: A2,B3,D1

Return Type String

Default "A1,B2"

Examples `SMC.EcalOrientation (1) = "A2,B1"`

C++ Syntax `HRESULT put_EcalOrientation(long IModuleNum, BSTR orientation);`
`HRESULT get_EcalOrientation(long IModuleNum, BSTR *orientation);`

Interface SMCType

EcalOrientation1Port Property

Description	For Mixer Characterization ONLY Specifies which port of the ECal module is connected to which port of the PNA for the <u>Do1PortECAL</u> property when the <u>AutoOrient</u> property = False.
VB Syntax	<code>VMC.EcalOrientation1Port (mod) = value</code>
Variable	(Type) - Description
<i>VMC</i>	<u>VMCType</u> (object)
<i>mod</i>	(Long) 1 - Use ECAL Module for the calibration.
<i>value</i>	(string) - Choose from: "A1" - ECAL module port A is connected to PNA port 1 "B1" - ECAL module port A is connected to PNA port 1
Return Type	String
Default	"A1" If anything other than port 1 is specified, "B1" will be used. For example, if "A2" is specified, "B1" is used.
Examples	<code>VMC.EcalOrientation1Port(1) = "B1"</code>
C++ Syntax	HRESULT put_EcalOrientation1Port(long IModuleNum, BSTR orientation); HRESULT get_EcalOrientation1Port(long IModuleNum, BSTR
Interface	VMCType

EcalOrientation2Port Property

Description Specifies which port of the ECal module is connected to which port of the PNA for the Do2PortECAL property when the AutoOrient property = False.

VB Syntax `VMC.EcalOrientation2Port (mod) = value`

Variable **(Type) - Description**

VMC VMCType (**object**)

mod (Long) Module being used for the calibration.
Choose from 1 or 2.

value **(string)** -Format this parameter in the following manner:
Aw,Bx,Cy,Dz
where

- A, B, C, and D are literal ports on the ECAL module
- w,x,y, and z are substituted for PNA port numbers to which the ECAL module port is connected.

Ports of the module which are not used are omitted from the string.

For example, on a 4-port ECal module with

- port A connected to PNA port 2
- port B connected to PNA port 3
- port C not connected
- port D connected to PNA port 1

the string would be: A2,B3,D1

Return Type String

Default "A1,B2"

Examples `VMC.EcalOrientation1Port(1) = "A2,B1"`

C++ Syntax `HRESULT put_EcalOrientation2Port(long IModuleNum, BSTR orientation);`
`HRESULT get_EcalOrientation2Port(long IModuleNum, BSTR *orientation);`

Interface VMCType

ECALPortMapEx Property

Description	This property replaces <u>ECALPortMap Property</u> Specifies which ports of the ECal module are connected to which ports of the PNA for the <u>DoECAL1PortEx</u> and <u>DoECAL2PortEx</u> methods when the <u>OrientECALModule</u> property = False.
VB Syntax	<i>cal</i> . ECALPortMapEx (<i>module</i>) = <i>value</i>
Variable	(Type) - Description
<i>cal</i>	A Calibrator (object)
<i>module</i>	(long integer) Optional argument. ECal module. Choose from modules 1 through 8 Use <u>IsECALModuleFoundEx</u> to determine the number of modules connected to the PNA Use <u>GetECALModuleInfoEx</u> to return the model and serial number of each module.
<i>value</i>	(string) -Format this parameter in the following manner: Aw,Bx,Cy,Dz where <ul style="list-style-type: none"> • A, B, C, and D are literal ports on the ECAL module • w,x,y, and z are substituted for PNA port numbers to which the ECAL module port is connected. Ports of the module which are not used are omitted from the string. For example, on a 4-port ECal module with <ul style="list-style-type: none"> • port A connected to PNA port 2 • port B connected to PNA port 3 • port C not connected • port D connected to PNA port 1 the string would be: A2,B3,D1 DoECAL1PortEx or DoECAL2PortEx methods will fail if the port numbers passed to those methods are not in the string of this property and <u>OrientECALModule</u> property = False.
Return Type	String
Default	Not Applicable

Examples `Dim cal As Calibrator
Dim sPortMap As String
Set cal = PNAapp.ActiveChannel.Calibrator
cal.ECALPortMapEx = "a2,b1" 'Write
sPortMap = cal.ECALPortMap 'Read`

C++ Syntax `HRESULT put_ECALPortMapEx(long moduleNumber, BSTR strPortMap);
HRESULT get_ECALPortMapEx(long moduleNumber, BSTR *strPortMap);`

Interface ICalibrator4

ElecDelayMedium Property

Description Sets or returns the electrical delay medium.

VB Syntax *meas.ElecDelayMedium = value*

Variable (Type) - Description

meas A Measurement **(object)**

value **(enum NACalStandardMedium)** choose from

0 - naCoax

1 - naWaveGuide

Return Type NACalStandardMedium

Default Not Applicable

Examples `Print meas.ElecDelayMedium 'prints the value of the electrical delay medium`

C++ Syntax `HRESULT get_ElecDelayMedium(tagNACalStandardMedium *pVal);`
`HRESULT put_ElecDelayMedium(tagNACalStandardMedium newVal);`

Interface IMeasurement2

ElectricalDelay Property

Description Sets the Electrical Delay for the active channel.

VB Syntax `meas.ElectricalDelay = value`

Variable (Type) - Description

`meas` A Measurement (**object**)

`value` (**double**) - Electrical Delay in seconds. Choose any number between **-9.99** and **9.99**

Return Type Double

Default 0

Examples `meas.ElectricalDelay = 1e-3 'Write`

`edelay = meas.ElectricalDelay 'Read`

C++ Syntax HRESULT get_ElectricalDelay(double *pVal)
HRESULT put_ElectricalDelay(double newVal)

Interface IMeasurement

Embed4PortA Property

Description Returns the PNA port number associated with 'a' based on the device topology.

To see 'a' for all topologies, and to specify the port connections, use [Embed4PortList Property](#)

Specify topology using [Embed4PortTopology Property](#)

VB Syntax *value* = *fixture*.**Embed4PortA**

Variable **(Type) - Description**

value (Short Integer) Variable to store the returned PNA port number.

fixture A [Fixturing \(object\)](#)

Return Type Integer

Default Not Applicable

Examples `value = fixture.Embed4PortA 'Read`

C++ Syntax HRESULT get_Embed4PortA(short *portA);

Interface IFixturing2

Embed4PortB Property

- Description** Returns the PNA port number associated with '**b**' based on the device topology.
To see '**b**' for all topologies, and to specify the port connections, use [Embed4PortList Property](#).
Specify topology using [Embed4PortTopology Property](#)
- VB Syntax** `value = fixture.Embed4PortB`
- Variable** **(Type) - Description**
- `value` (Short Integer) Variable to store the returned PNA port number.
- `fixture` A [Fixturing \(object\)](#)
- Return Type** Integer
- Default** Not Applicable
- Examples** `value = fixture.Embed4PortB 'Read`
- C++ Syntax** HRESULT get_Embed4PortB(short *portB);
- Interface** IFixturing2

Embed4PortC Property

- Description** Returns the PNA port number associated with 'c' based on the device topology.
To see 'c' for all topologies, and to specify the port connections, use [Embed4PortList Property](#).
Specify topology using [Embed4PortTopology Property](#)
- VB Syntax** `value = fixture.Embed4PortC`
- Variable** **(Type) - Description**
- `value` (Short Integer) Variable to store the returned PNA port number.
- `fixture` A [Fixturing \(object\)](#)
- Return Type** Integer
- Default** Not Applicable
- Examples** `value = fixture.Embed4PortC 'Read`
- C++ Syntax** `HRESULT get_Embed4PortC(short *portC);`
- Interface** IFixturing2

Embed4PortD Property

- Description** Returns the PNA port number associated with '**d**' based on the device topology.
To see '**d**' for all topologies, and to specify the port connections, use [Embed4PortList Property](#).
Specify topology using [Embed4PortTopology Property](#)
- VB Syntax** `value = fixture.Embed4PortD`
- Variable** **(Type) - Description**
- `value` (Short Integer) Variable to store the returned PNA port number.
- `fixture` A [Fixturing \(object\)](#)
- Return Type** Integer
- Default** Not Applicable
- Examples** `value = fixture.Embed4PortD 'Read`
- C++ Syntax** `HRESULT get_Embed4PortD(short *portD);`
- Interface** IFixturing2

Embed4PortList Property




Description Specifies the PNA port connections for ALL topologies. The port assignment is dependent on the DUT topology. All four port numbers are required. However, for:

- Topology A, only the first **two** arguments are valid,
- Topology B, only the first **three** arguments are valid,
- Topology C, **ALL** arguments are valid.

Specify topology using [Embed4PortTopology Property](#).

Read the port assignments using the following commands. A, B, C, and D, refer to the port; NOT the topology.

- [Embed4PortA Property](#)
- [Embed4PortB Property](#)
- [Embed4PortC Property](#)
- [Embed4PortD Property](#)

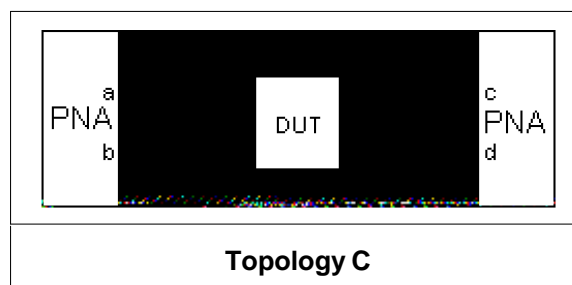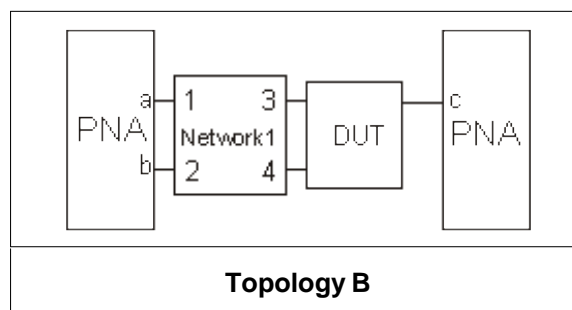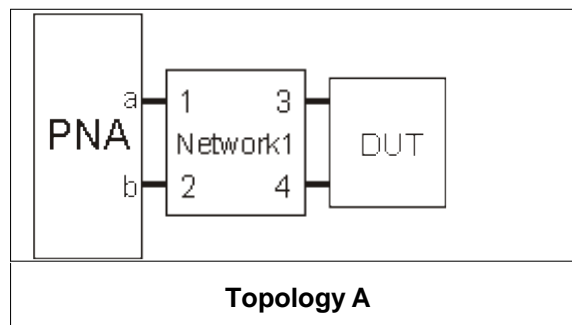

VB Syntax `fixture.Embed4PortList = p1, p2, p3, p4`

Variable **(Type) - Description**

`fixture` A Fixturing **(object)**

`p1` PNA Port number assigned to **a** in above graphic.

`p2` PNA Port number assigned to **b** in above graphic.

`p3` PNA Port number assigned to **c** in above graphic.

`p4` PNA Port number assigned to **d** in above graphic.

Return Type Four Integers

Default 1,2,3,4

Examples `fixture.4PortNetworkTopoCPorts = 4,3,2,1 'Write`

C++ Syntax HRESULT put_4PortNetworkTopoCPorts(short ChannelNum, short pPortA, short pPortB, short pPortC, short pPortD)

Interface IFixturing2

Embed4PortNetworkFilename Property

Description Specifies the 4-port touchstone file (*.s4p) in which the network to embed or de-embed resides. If the specified file does not exist, an error occurs when type command is sent.

Following this command, send [Embed4PortNetworkMode Property](#).

Note: This command affects ALL measurements on the channel.

VB Syntax *fixture*.Embed4PortNetworkFilename(*netNum*) = *value*

Variable (Type) - Description

fixture A [Fixturing](#) (**object**)

netNum (**Integer**) Network position. Choose from **1** or **2**. See [Embed4PortTopology Property](#)

value (**String**) Full path, file name, and extension (.s4P) of the circuit.

Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents"

Return Type String

Default Not Applicable

Examples `fixture.Embed4PortNetworkFilename(2) = "C:\Program Files\Agilent\Network Analyzer\Documents\myFile.s4p" 'Write`

`value = fixture.Embed4PortNetworkFilename(1) 'Read`

C++ Syntax HRESULT get_Embed4PortNetworkFilename(short networkNum, BSTR *filename);
 HRESULT put_Embed4PortNetworkFilename(short networkNum, BSTR filename);

Interface IFixturing2

Embed4PortNetworkMode Property

Description Specify the type of processing to take place on the specified 4-port network. First specify the network filename with [FSim.Embed4PortNetworkFilename Property](#).

VB Syntax `fixture.Embed4PortNetworkMode(netNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing \(object\)](#)

`netNum` **(Integer)** Network position. Choose from **1** or **2**. See [Embed4PortTopology Property](#)

`value` **(Enum as NA4PortEmbedNetworkMode)** Processing mode. Choose from:

- **0** or **naNO_NETWORK** - The same as disabling.
- **1** or **naEMBED_NETWORK** - Add Network circuit.
- **2** or **naDEEMBED_NETWORK** - Remove Network circuit

Return Type Enum

Default naNO_NETWORK

Examples `fixture.Embed4PortNetworkMode(1) = naNO_NETWORK 'Write`

`value = fixture.Embed4PortNetworkMode(2) 'Read`

C++ Syntax `HRESULT get_Embed4PortNetworkMode(short networkNum, tagNA4PortEmbedNetworkMode *eVal);`
`HRESULT put_Embed4PortNetworkMode(short networkNum, tagNA4PortEmbedNetworkMode eVal);`

Interface IFixturing2

Embed4PortState Property

Description Turns ON or OFF 4-port Network embedding for all ports on the channel.

VB Syntax `fixture.Embed4PortState = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`value` (**Boolean**)

False - Turns Embedding OFF

True - Turns Embedding ON

Return Type Boolean

Default False (OFF)

Examples `fixture.Embed4PortState = 0 'Write`

`value = fixture.Embed4PortState 'Read`

C++ Syntax HRESULT get_Embed4PortState(VARIANT_BOOL *pVal)
HRESULT put_Embed4PortState(VARIANT_BOOL newVal)

Interface IFixturing2

Embed4PortTopology Property

Description Specifies the PNA / DUT topology. [Learn more about these and other PNA/DUT configurations.](#)

VB Syntax `fixture.Embed4PortTopology = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (object)

`value` **(Enum as NA4PortEmbedTopology)** PNA / DUT topology. Choose from:

0 or `naTOPOLOGY_A` - 2 PNA/DUT Ports

1 or `naTOPOLOGY_B` - 3 PNA/DUT Ports

2 or `naTOPOLOGY_C` - 4 PNA/DUT Ports

Return Type Enum

Default `naTOPOLOGY_A` (2 PNA/DUT Ports)

Examples `fixture.Embed4PortTopology = naTOPOLOGY_A 'Write`

`value = fixture.Embed4PortTopology 'Read`

C++ Syntax `HRESULT get_Embed4PortTopology(tagNA4PortEmbedTopology *eVal);`
`HRESULT put_Embed4PortTopology(tagNA4PortEmbedTopology eVal);`

Interface IFixturing2

Enabled Property

Description Turns ON/OFF the port switching and control line output of the specified E5091A. This setting affects all channels in use by the specified testset.

If the specified testset is not connected to USB or not ON, then setting Enabled = True will report an error. All other properties of the object can be set when the testset is not connected.

VB Syntax `testsets(1).Enabled = value`

Variable **(Type) - Description**

`testsets(1)` An item from Testsets **(collection)**
Learn how to identify a testset in the collection.

`value` **(Boolean)**

ON(1) Turns switching ON.

OFF (0) Turns switching OFF.

Return Type Boolean

Default 0

Examples [See Example Program](#)

C++ Syntax HRESULT get_Enabled(VARIANT_BOOL *state);
HRESULT put_Enabled(VARIANT_BOOL state);

Interface IE5091Testsets

ErrorCorrection Property

Description Sets (or returns) error correction ON or OFF for the measurement.

VB Syntax `meas.ErrorCorrection = value`

Variable (Type) - Description

`meas` A Measurement (**object**)

`value` **(boolean)**
0 - Turns error correction OFF
1 - Turns error correction ON

Return Type Boolean

Default Not Applicable

Examples `meas.ErrorCorrection = 1 'Write`

`errcorr = meas.ErrorCorrection 'Read`

C++ Syntax HRESULT put_ErrorCorrection (VARIANT_BOOL bState)
HRESULT get_ErrorCorrection (VARIANT_BOOL *bState)

Interface IMeasurement

ErrorCorrection (Channel) Property

Description Attempts to sets error correction ON or OFF for all of the measurements on the channel. This setting may not be successful for some measurements because of the Cal Set currently in place may not contain the appropriate calibration data. To read the error correction state for a measurement, use Error Correction Property.

VB Syntax `chan.ErrorCorrection = value`

Variable (Type) - Description

chan A Channel (**object**)

value (**boolean**)

0 - Turns error correction OFF

1 - Turns error correction ON

Return Type Boolean

Default Not Applicable

Examples `chan.ErrorCorrection = 1`

C++ Syntax HRESULT put_ErrorCorrection (VARIANT_BOOL bState)

Interface IChannel7

Write/Read

ExternalALC Property

Description Sets or returns the source of the analyzer leveling control.

VB Syntax `app.ExternalALC = value`

Variable (Type) - Description

app An Application (**object**)

value (**boolean**) - Choose from:
True (or 1) - Leveling control supplied through the rear panel.
False (or 0) - Leveling control supplied inside the analyzer

Return Type Boolean

Default 0

Examples `app.ExternalALC = True 'Write`

`extALC = app.ExternalALC 'Read`

C++ Syntax HRESULT get_ExternalALC(VARIANT_BOOL *pVal)
HRESULT put_ExternalALC(VARIANT_BOOL newVal)

Interface IApplication

Write/Read.

ExternalTriggerConnectionBehavior Property

- Description** Configures the external triggering signal for the PNA.
- TriggerSouce Property is automatically set to External when **ExternalTriggerConnectionBehavior** is sent.
- Edge triggering is only available on some PNA models. For more information, see External Triggering.
- VB Syntax** `trigsetup.ExternalTriggerConnectionBehavior (conn) = value`
- Variable** **(Type) - Description**
- trigsetup* A TriggerSetup (object)
- conn* **(enum NATriggerConnection)** Rear Panel connector to send or receive trigger signals. Choose from:
- Only one of the input connectors is active at a time. When a command is sent to one, the PNA automatically makes the other INACTIVE.
- 0 - **naTriggerConnectionAUXT** Trigger IN from rear-panel AUX IO connector Pin 19
 - 1 - **naTriggerConnectionBNC1** Trigger IN from rear-panel Trigger IN BNC connector
 - 2 - **naTriggerConnectionBNC2** Trigger OUT to rear-panel Trigger OUT BNC connector. Only useful in point sweep mode.
 - 3 - **naTriggerConnectionMATH** Trigger IN from rear-panel Material Handler connector Pin 18
- value* **(enum NAExternalTriggerBehavior) -**
- 0 - **naTriggerInactive** - Disables the specified connector.
- Choose from ONLY 1 through 4** when <conn> is set to either **naTriggerConnectionBNC1** or **naTriggerConnectionAUXT**
- 1 - **naTriggerInEdgeNegative** - Triggers the PNA when receiving a negative going signal
 - 2 - **naTriggerInEdgePositive** - Triggers the PNA when receiving a positive going signal
 - 3 - **naTriggerInLevelLow** - Triggers the PNA when receiving a low level signal
 - 4 - **naTriggerInLevelHigh** - Triggers the PNA when receiving a High-level signal
- Choose from ONLY 5 through 8** when <conn> is set to **naTriggerConnectionBNC2**.
- In addition to sending this command, you must also use TriggerOutputEnabled Property to enable the BNC2 output.
- 5 - **naTriggerOutPulsePositiveAfter** - Sends a POSITIVE going TTL pulse at the END of each point during the sweep.
 - 6 - **naTriggerOutPulsePositiveBefore** - Sends a POSITIVE going TTL pulse at the START of each point during the sweep.
 - 7 - **naTriggerOutPulseNegativeAfter** - Sends a NEGATIVE going TTL pulse at the END of each point during the sweep.
 - 8 - **naTriggerOutPulseNegativeBefore** - Sends a NEGATIVE going TTL pulse at the START of

each point during the sweep.

Return Type Enum as NAExternalTriggerBehavior

Default BNC1 = naTriggerInactive
BNC2 = naTriggerInactive
AUXT = naTriggerInLevelHigh

When Output is enabled

BNC1 = naTriggerInactive
BNC2 = naTriggerOutPulsePositiveAfter
AUXT = naTriggerInLevelHigh

Examples `trigsetup.ExternalTriggerConnectionBehavior (naTriggerConnectionAUXT) = naTriggerInLevelLow 'Write`

```
trigBehav = trigsetup.ExternalTriggerConnectionBehavior
(naTriggerConnectionAUXT) 'Read
```

C++ Syntax HRESULT get_ExternalTriggerConnectionBehavior(tagNATriggerConnection connection,tagNAExternalTriggerBehavior *trigger);
HRESULT put_ExternalTriggerConnectionBehavior(tagNATriggerConnection connection,tagNAExternalTriggerBehavior trigger);

Interface ITriggerSetup

ExternalTriggerDelay Property

Description Sets and reads the trigger delay for all measurements in the CHANNEL. This delay is only applied while in `app.Source = naTriggerSourceExternal` and `trigsetup.Scope = naChannelTrigger`. After an external trigger is applied, the start of the sweep is delayed for the specified delay value plus any inherent latency.

To apply a trigger delay for all channels (Global), use [TriggerDelay Property](#).

VB Syntax `chan.ExternalTriggerDelay = value`

Variable (Type) - Description

chan A [Channel](#) (object)

value **Double**- Trigger delay value in seconds. Range is from 0 to 107 seconds

Return Type Double

Default 0

Examples `chan.ExternalTriggerDelay = .003 'Write`

`delay = chan.ExternalTriggerDelay 'Read`

C++ Syntax HRESULT get_ExternalTriggerDelay(double *delay);
HRESULT put_ExternalTriggerDelay(double delay)

Interface IChannel6

Read-only

FilterBW Property

Description Returns the results of the SearchBandwidth method.

VB Syntax `filtBW = meas.FilterBW`

Variable **(Type) - Description**

`filtBW` **(single)** - Variable to store bandwidth data

`meas` A Measurement **(object)**

Return Type Single

Default Not applicable

Examples `filterBW = meas.FilterBW 'Read`

C++ Syntax HRESULT get_FilterBW(float* bw)

Interface IMeasurement

Read-only

FilterCF Property

Description Returns the Center Frequency result of the SearchBandwidth method.

VB Syntax `filtCF = meas.FilterCF`

Variable **(Type) - Description**

`filtCF` **(double)** - Variable to store bandwidth CF data

`meas` A Measurement **(object)**

Return Type Double

Default Not applicable

Examples `filtCF = meas.FilterCF 'Read`

C++ Syntax HRESULT get_FilterCF(double* centerFrequency)

Interface IMeasurement

Read-only

FilterLoss Property

Description Returns the Loss value of the SearchBandwidth method.

VB Syntax `filtLoss = meas.FilterLoss`

Variable (Type) - Description

`filtLoss` **(single)** - Variable to store bandwidth Loss data

`meas` A Measurement **(object)**

Return Type Single

Default Not applicable

Examples `filterLoss = meas.FilterLoss 'Read`

C++ Syntax HRESULT get_FilterLoss(float* loss)

Interface IMeasurement

Read-only

FilterQ Property

Description Returns the Q (quality factor) result of the SearchBandwidth method.

VB Syntax `filtQ = meas.FilterQ`

Variable (Type) - Description

`filtQ` **(single)** - Variable to store bandwidth Q data

`meas` A Measurement **(object)**

Return Type Single

Default Not applicable

Examples `filtQ = meas.FilterQ 'Read`

C++ Syntax HRESULT get_FilterQ(float* quality)

Interface IMeasurement

FirmwareMajorRevision Property

Description Returns the major firmware revision number as an integer. For example, given a firmware revision number A.03.30, this command returns 3.

VB Syntax `value = cap.FirmwareMajorRevision`

Variable **(Type) - Description**

`value` (Long) - Variable to store the returned integer value of the firmware revision number.

`cap` A [Capabilities](#) **(object)**

Return Type Long

Default Not Applicable

Examples `value = cap.FirmwareMajorRevision 'Read`

C++ Syntax HRESULT get_FirmwareMajorRevision(long * majorRev);

Interface ICapabilities

FirmwareMinorRevision Property

Description Returns the minor firmware revision number as an integer. For example, given a firmware revision number A.03.30, this command returns 30.

VB Syntax `value = cap.FirmwareMinorRevision`

Variable **(Type) - Description**

`value` (Long) - Variable to store the returned decimal value of the firmware revision number.

`cap` A [Capabilities](#) **(object)**

Return Type Long

Default Not Applicable

Examples `value = cap.FirmwareMinorRevision 'Read`

C++ Syntax HRESULT get_FirmwareMinorRevision(long * minorRev);

Interface ICapabilities

FirmwareSeries Property

Description Returns the alpha portion of the firmware revision number. For example, given a firmware revision number A.03.30, this command returns A.

VB Syntax `value = cap.FirmwareSeries`

Variable **(Type) - Description**

`value` (String) - Variable to store the returned alpha value of the firmware revision number.

`cap` A [Capabilities](#) **(object)**

Return Type String

Default Not Applicable

Examples `value = cap.FirmwareSeries 'Read`

C++ Syntax HRESULT get_FirmwareSeries(BSTR * series);

Interface ICapabilities

FixturingState Property

Description Turns all three fixturing functions (de-embedding, port matching, impedance conversion) ON or OFF for all ports on the specified channel. This does NOT affect port extensions.

VB Syntax *fixture.FixturingState* = *value*

Variable (Type) - Description

fixture A [Fixturing](#) (object)

value (boolean)

True or **1** - Turns Fixturing ON

False or **0** - Turns Fixturing OFF

Return Type Boolean

Default False

Examples `fixture.FixturingState = True 'Write`

`value = fixture.FixturingState 'Read`

C++ Syntax HRESULT get_FixturingState(VARIANT_BOOL *pVal)
HRESULT put_FixturingState(VARIANT_BOOL newVal)

Interface IFixturing

Read-only

FootSwitch Property

Description Reads the Footswitch Input (pin 20 of the AUX IO connector).

VB Syntax *value* = *AuxIO.Footswitch*

Variable (Type) - Description

value **(boolean)** - Variable to store the returned value

False (0) -foot switch is released

True (1) - footswitch is depressed

AuxIO **(object)** - A Hardware Aux I/O object

Return Type Boolean

Default True (1)

Examples `fs = aux.Footswitch`

C++ Syntax HRESULT get_FootSwitch (VARIANT_BOOL* State);

Interface IHWAuxIO

FootswitchMode Property

Description	Determines what occurs when the footswitch is pressed. For more information see the FootSwitch In pin description in the Auxiliary IO connector.
VB Syntax	<i>AuxIo.FootSwitchMode</i> = <i>value</i>
Variable	(Type) - Description
<i>value</i>	(enum NAFootSwitchMode)
	0 - nalignoreFootswitch - Footswitch presses are ignored.
	1 - naSweepTrigger - Footswitch presses trigger a sweep. The PNA must be in Manual Trigger Mode.
	2 - naRecallNextState - Footswitch presses recall an instrument state. When more than one state is available, then each footswitch press recalls the next state, then starts over from the beginning. It is possible for a recalled state to override the current mode. If the recalled state is IGNore, then mode changes and additional footswitch presses are ignored.
	3 - naRunMacro - Footswitch presses load and run a macro. When more than one macro is available, then each footswitch press loads and runs the next macro, then starts over from the beginning. It is possible for a Macro to override the current mode. If the macro contains a Preset, then the mode changes to the default setting IGNore and additional footswitch presses are ignored.
<i>AuxIO</i>	(object) - A Hardware Aux I/O object
Return Type	NAFootSwitchMode
Default	0 - nalignoreFootswitch
Examples	<code>auxIo.FootSwitchMode = naIgnoreFootSwitch 'Write</code>
C++ Syntax	HRESULT get_FootSwitchMode(NAFootSwitchMode *pFootSwitchMode) HRESULT put_FootSwitchMode(NAFootSwitchMode newFootSwitchMode)
Interface	IHWAuxIO3

Format Property (marker)

Description Sets (or returns) the format of the marker.

VB Syntax `mark.Format = value`

Variable **(Type) - Description**

mark A Marker (**object**)

value (**enum NAMarkerFormat**) - Choose from:

- 0 - naMarkerFormat_LinMag
- 1 - naMarkerFormat_LogMag
- 2 - naMarkerFormat_Phase
- 3 - naMarkerFormat_Delay
- 4 - naMarkerFormat_Real
- 5 - naMarkerFormat_Imaginary
- 6 - naMarkerFormat_SWR
- 7 - naMarkerFormat_LinMagPhase
- 8 - naMarkerFormat_LogMagPhase
- 9 - naMarkerFormat_ReallImaginary
- 10 - naMarkerFormat_ComplexImpedance
- 11 - naMarkerFormat_ComplexAdmittance

Return Type NAMarkerFormat

Default 1 - naMarkerFormat_LogMag

Examples `mark.Format = naMarkerFormat_SWR 'Write`
`fmt = mark.Format 'Read`

C++ Syntax HRESULT get_Format(tagNAMarkerFormat *pVal)
 HRESULT put_Format(tagNAMarkerFormat newVal)

Interface IMarker

Frequency Property

Description Sets or returns the frequency associated with a PowerSensorCalFactorSegment
or

Sets or returns the frequency associated with a PowerLossSegment.

VB Syntax *object.Frequency = value*

Variable (Type) - Description

object **(object)** - PowerSensorCalFactorSegment or PowerLossSegment

value **(double)** – Frequency in units of Hz. This can be any non-negative value (limited by the maximum value of double).

Return Type Double

Default 0

Examples `seg.Frequency = 6e9 'Write`
`freq = seg.Frequency 'Read`

C++ Syntax HRESULT put_Frequency(double newVal);
HRESULT get_Frequency(double *pVal);

Interface IPowerSensorCalFactorSegment
IPowerLossSegment

Write/Read

FrequencySpan Property

Description Sets or returns the frequency span of the channel.
Sets or returns the frequency span of the segment.

VB Syntax `object.FrequencySpan = value`

Variable **(Type) - Description**

object A Channel **(object)**
or
A Segment **(object)**

value **(double)** - Frequency span in Hertz. Choose any number between the **minimum** and **maximum** frequencies of the analyzer.

Return Type Double

Default Full frequency span of the analyzer

Examples `chan.FrequencySpan = 4.5e9 'sets the frequency span of a linear sweep for the channel object -Write`

`freqspan = chan.FrequencySpan 'Read`

C++ Syntax HRESULT get_FrequencySpan(double *pVal)
HRESULT put_FrequencySpan(double newVal)

Interface IChannel
ISegment

Read / Write

FrequencyList Property

Description

VB Syntax `guidedCal.FrequencyList = value`

Variable **(Type) - Description**

guidedCal GuidedCalibration (object)

value (Variant) -

Return Type Variant

Default

Examples

```
Dim value
value = MySMC.FrequencyList
```

C++ Syntax HRESULT get_FrequencyList(Variant *freqList)
HRESULT put_FrequencyList(Variant freqList)

Interface IGuidedCalibration

FrequencyOffsetDivisor Property

Description Specifies (along with [FrequencyOffsetMultiplier](#)) the value to multiply by the stimulus.
See other [Frequency Offset](#) properties

VB Syntax `object.FrequencyOffsetDivisor = value`

Variable (Type) - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

value (**Double**) - Divisor value. Range is 1 to 1000

Return Type Double

Default 1

Examples `chan.FrequencyOffsetDivisor = 2 'Write`

```
fOffsetDiv = chan.FrequencyOffsetDivisor 'Read
```

C++ Syntax HRESULT get_FrequencyOffsetDivisor(double*pval)
HRESULT put_FrequencyOffsetDivisor(double newVal)

Interface IChannel2

|CalSet3

FrequencyOffsetFrequency Property

Description Specifies an absolute offset frequency in Hz. For mixer measurements, this would be the LO frequency. See other [Frequency Offset](#) properties.

VB Syntax *object.FrequencyOffsetFrequency = value*

Variable **(Type) - Description**

object Channel (**object**)

or

CalSet (**object**) - Read-only property

value (**Double**) - Offset value. Range is +/- 1000 GHz. (Offsets can be positive or negative.)

Return Type Double

Default 0 Hz

Examples `chan.FrequencyOffsetFrequency = 2 'Write`

`fOffsetFreq = chan.FrequencyOffsetFrequency 'Read`

C++ Syntax HRESULT get_FrequencyOffsetFrequency(double*pval)
 HRESULT put_FrequencyOffsetFrequency(double newVal)

Interface IChannel2

|CalSet3

FrequencyOffsetMultiplier Property

Description Specifies (along with [FrequencyOffsetDivisor](#)) the value to multiply by the stimulus. See other [Frequency Offset](#) properties.

VB Syntax *object.FrequencyOffsetMultiplier = value*

Variable (Type) - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

value (**Double**) - Multiplier value. Range is 1 to 1000

Return Type Double

Default 1

Examples `chan.FrequencyOffsetMultiplier = 2 'Write`

`fOffsetMult = chan.FrequencyOffsetMultiplier 'Read`

C++ Syntax HRESULT get_FrequencyOffsetMultiplier (double*pval);
HRESULT put_FrequencyOffsetMultiplier (double newVal);

Interface IChannel2

|CalSet3

FrequencyOffsetCWOverride Property

Description Establishes a fixed (CW) stimulus frequency while measuring the Response over a swept frequency range. For example, a fixed-frequency PNA stimulus may be applied to the RF input of a mixer whose local oscillator (LO) is being swept. Because the IF output of the mixer will be swept, the PNA receivers must also be swept.

See other [Frequency Offset](#) properties.

VB Syntax *object*.**FrequencyOffsetCWOverride** = *value*

Variable **(Type)** - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

value **(Enum as NaStates)** - Choose from:

naOFF (0) - Turns CW override OFF

naON (1) - Turns CW override ON

Return Type Enum

Default 0 Hz

Examples `chan.FrequencyOffsetCWOverride = 1 'Write`

`fOffsetOV = chan.FrequencyOffsetCWOverride 'Read`

C++ Syntax HRESULT get_FrequencyOffsetCWOverride (tagNAStates *pstate)
 HRESULT put_FrequencyOffsetCWOverride (tag NAStates newState)

Interface IChannel2
 |CalSet3

FrequencyOffsetState Property

Description Enables Frequency Offset on ALL measurements that are present on the active channel. This immediately causes the source and receiver to tune to separate frequencies. The receiver frequencies are specified with other channel and offset settings. To make the stimulus settings, use Channel Start, Stop Frequency properties. See other [Frequency Offset](#) properties.

Tip: To avoid unnecessary errors, first make other frequency offset settings. Then turn Frequency Offset ON.

VB Syntax *object*.**FrequencyOffsetState** = *value*

Variable **(Type)** - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

value **(Enum as NaStates)** - Choose from:

naOFF (0) - Turns Frequency Offset OFF

naON (1) - Turns Frequency Offset ON

Return Type Enum

Default naOFF (0)

Examples `chan.FrequencyOffsetState = True 'Write`

`Foffset = chan.FrequencyOffsetState 'Read`

C++ Syntax HRESULT FrequencyOffsetState (tag NAStates *pState);
HRESULT FrequencyOffsetState (tag NAStates newState)

Interface IChannel2
|CalSet3

Shape Property

Description Specifies the shape of the gate filter.

VB Syntax `gat.Shape = value`

Variable **(Type) - Description**

`gat` A Gating **(object)**

`value` **(enum NAGateShape)** - Choose from:

0 - naGateShapeMaximum

1 - naGateShapeWide

2 - naGateShapeNormal

3 - naGateShapeMinimum

Return Type NAGateShape

Default 2 - Normal

Examples `gat.Shape = naGateShapeMaximum 'Write`

`filterShape = gat.Shape 'Read`

C++ Syntax HRESULT get_Shape(tagNAGateShape *pVal)
HRESULT put_Shape(tagNAGateShape newVal)

Interface IGating

Write/Read

Type Property

Description Specifies the type of gate filter used.**VB Syntax** `gat.Type = value`**Variable** **(Type) - Description***gat* A Gating (**object**)*value* (**enum NAGateType**) - Choose from:**0 - naGateTypeBandpass** - Includes (passes) the range between the start and stop times.**1 - naGateTypeNotch** - Excludes (attenuates) the range between the start and stop times.**Return Type** NAGateType**Default** Bandpass**Examples** `gate.Type = naGateTypeNotch 'Write``filterType = gate.Type 'Read`**C++ Syntax** HRESULT get_Type(tagNAGateType *pVal)
HRESULT put_Type(tagNAGateType newVal)**Interface** IGating

GPIBAddress Property

Description Sets and returns the PNA GPIB address bus.

VB Syntax `app.GPIBAddress (bus) = value`

Variable **(Type) - Description**

app An Application (**object**)

bus (Short Integer) GPIB bus. MUST be set to 0.

value (Short Integer) GPIB Address on the PNA. Choose a value between 0 and 30.

Return Type Short Integer

Default 16

Examples `address=app.GPIBAddress(0) 'Read`

`app.GPIBAddress(0)=16 'Write`

C++ Syntax `HRESULT get_GPIBAddress(short busIndex, short* address);`
`HRESULT put_GPIBAddress(short busIndex,short address);`

Interface IApplication8

GPIBMode Property

Description Changes the analyzer to a GPIB system controller or a talker/listener on the bus. The analyzer must be the controller if you want to use it to send commands to other instruments. The analyzer must be a talker/listener if you want to send it commands from another PC.

VB Syntax `app.GPIBMode value`

Variable **(Type) - Description**

app An Application (**object**)

value (**enum NAGPIBMode**) -Choose either:
0 - naTalkerListener - the analyzer is a talker / listener
1 - naSystemController - the analyzer is the system controller

Return Type Long Integer

Default 0 - naTalkerListener

Examples `app.GPIBMode = naTalkerListener 'Write`

`mode = app.GPIBMode 'Read`

C++ Syntax HRESULT get_GPIBMode(tagGPIBModeEnum* eGpibMode)
 HRESULT put_GPIBMode(tagGPIBModeEnum eGpibMode)

Interface IApplication

ID Property

Description Returns the test set ID number.

VB Syntax *value* = *testsets(1).ID*

Variable **(Type) - Description**

value (Long) variable to store the returned information.

testsets(1) An item from Testsets (**collection**)

Learn how to identify a testset in the collection.

Return Type Long Integer

Default Not Applicable

Examples `value = testset1.ID`

See Example Program

C++ Syntax HRESULT get_ID(long *idNumber);

Interface IE5091Testsets

Read-only

IDString Property

Description Returns the ID of the analyzer, including the Model number, Serial Number, and the Software revision number.

VB Syntax *value* = *app.IDString*

Variable (Type) - Description

app An Application (**object**)

value (**string**) - variable to contain the returned ID string

Return Type String

Default Not Applicable

Examples `id = app.IDString`

C++ Syntax HRESULT IDString(BSTR* IDString)

Interface IApplication

Write/Read

IFBandwidthOption Property

Description Enables the IFBandwidth to be set on individual sweep segments. This property must be set True **before** `seg.IFBandwidth = value` is sent. Otherwise, this command will be ignored.

VB Syntax `segs.IFBandwidthOption = value`

Variable (Type) - Description

`segs` A Segments collection (**object**)

`value` (**boolean**)

True - Enables variable IFBandwidth setting for segment sweep

False - Disables variable IFBandwidth setting for segment sweep

Return Type Boolean

Default False

Examples `segs.IFBandwidthOption = True 'Write`

`IFOption = IFBandwidthOption 'Read`

C++ Syntax HRESULT get_IFBandwidthOption(VARIANT_BOOL *pVal)
 HRESULT put_IFBandwidthOption(VARIANT_BOOL newVal)

Interface ISegments

Write/Read

IFBandwidth Property

Description Sets or returns the IF Bandwidth of the channel.
Sets or returns the IF Bandwidth of the segment.
Returns the IF Bandwidth used in the Cal Set

VB Syntax *object*.IFBandwidth = *value*

Variable (Type) - Description

object Channel **(object)**

or

Segment **(object)**

or

CalSet **(object)** - Read-only property

value **(double)** - IF Bandwidth in Hz. The list of valid IF Bandwidths is different depending on the PNA model. [\(Click to see the lists.\)](#) If an invalid number is specified, the analyzer will round up to the closest valid number.

Return Type Double

Default See [Preset IFBW](#) for your PNA model.

Examples `chan.IFBandwidth = 3e3 'sets the IF Bandwidth of for the channel object to 3 kHz. -Write`
`seg.IFBandwidth = 5 'sets the IF Bandwidth of the segment to 5 Hz. -Write`

`ifbw = chan.IFBandwidth -Read`

C++ Syntax HRESULT get_IFBandwidth(double *pVal);
HRESULT put_IFBandwidth(double newVal);

Interface IChannel
ISegment
|CalSet3

IFDenominator Property

Description Sets or returns the denominator value of the IF Fractional Multiplier.
Only applies to 2 stage mixers!

VB Syntax `mixer.IFDenominator = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(long)** IF Denominator value.

Return Type Long

Default 1

Examples `Print mixer.IFDenominator` 'prints the value of the IFDenominator

C++ Syntax HRESULT get_IFDenominator(long *pVal)
HRESULT put_IFDenominator(long newVal)

Interface IMixer

IFFilterSampleCount Property

Description Sets or retrieves the number of taps in the IF filter when the [IFFilterSource](#) property is set to `naIFFilterSourceManual`.

Note: An error will occur if this command is used on a PNA without option H08 installed.

VB Syntax `IfConfig.IFFilterSampleCount = value`

Variable **(Type) - Description**

IfConfig [IFConfiguration](#) (object)

value **(long)** – The IF filter sample count. The minimum and maximum allowed values for this property can vary by model number, but can be queried using the [MinimumIFFilterSampleCount](#) and [MaximumIFFilterSampleCount](#) properties.

Return Type Long Integer

Default PNA Model number dependent

Examples `App.ActiveChannel.IFConfiguration.IFFilterSampleCount = 200 'Write`

`variable = App.ActiveChannel.IFConfiguration.IFFilterSampleCount 'Read`

[See an example program](#)

C++ Syntax `HRESULT get_IFFilterSampleCount(long * pSampleCount);`
`HRESULT put_IFFilterSampleCount (long sampleCount);`

Interface `IIFConfiguration2`

IFFilterSamplePeriod Property

Description Sets or returns the IF filter sample period time. This time is only used if the [IFFilterSamplePeriodMode](#) is set to naManual.

Note: An error will occur if this command is used on a PNA without option H08 installed.

VB Syntax *IfConfig.IFFilterSamplePeriod = value*

Variable **(Type) - Description**

IfConfig [IFConfiguration](#) (object)

value **(double)** – The sample period time in seconds. Valid sample period times can be queried using the [IFFilterSamplePeriodList](#) property.

Return Type Double

Default PNA Model number dependent.

Examples `App.ActiveChannel.IFConfiguration.IFFilterSamplePeriod = .000006 'Write`

`variable = App.ActiveChannel.IFConfiguration.IFFilterSamplePeriod 'Read`

[See an example program](#)

C++ Syntax HRESULT get_IFFilterSamplePeriod(double * pSamplePeriod);
HRESULT put_IFFilterSamplePeriod (double samplePeriod);

Interface IIFConfiguration2

IFFilterSamplePeriodList Property

Description	Retrieves the list of available IF filter sample periods for the instrument. Note: An error will occur if this command is used on a PNA without option H08 installed.
VB Syntax	<i>variable</i> = <i>IfConfig</i> .IFFilterSamplePeriodList
Variable	(Type) - Description
<i>variable</i>	(Array) An array of permissible values that can be passed to the <u>IFFilterSamplePeriod</u> property.
<i>IfConfig</i>	<u>IFConfiguration</u> (object)
Return Type	Array
Default	Not applicable
Examples	<pre>Dim Variable Variable = App.ActiveChannel.IFConfiguration.IFFilterSamplePeriodList 'Read MsgBox "First IF Sample Period Value: " & Variable(0)</pre> <p>See an example program</p>
C++ Syntax	HRESULT get_IFFilterSamplePeriodList(SAFEARRAY ** ppSamplePeriodList);
Interface	IIFConfiguration2

IFFilterSamplePeriodMode Property

Description Sets or returns the IF filter sample period mode.

Note: An error will occur if this command is used on a PNA without option H08 installed.

VB Syntax *IfConfig.IFFilterSamplePeriodMode = value*

Variable (Type) - Description

IfConfig IFConfiguration (object)

value **(enum NAModes) -**

0 - naAuto - IF filter sample period is chosen automatically.

1 - naManual - the IF filter sample period is the value specified by the IFSamplePeriod property.

Return Type NAModes

Default 0 - naAuto

Examples `App.ActiveChannel.IFConfiguration.IFFilterSamplePeriodMode = naAuto`
`'Write`

`variable = App.ActiveChannel.IFConfiguration.IFFilterSamplePeriodMode`
`'Read`

[See an example program](#)

C++ Syntax HRESULT get_IFFilterSamplePeriodMode(tagNAModes * pMode);
HRESULT put_IFFilterSamplePeriodMode (tagNAModes mode);

Interface IIFConfiguration2

IFFilterSource Property

Description Sets or retrieves type of IF filter to be used.

Note: An error will occur if this command is used on a PNA without option H08 installed.

VB Syntax *IfConfig.IFFilterSource = value*

Variable **(Type) - Description**

object IFConfiguration (object)

value **(NAIFFilterSource)** – The type of filter to use. Choose from:

naIFFilterSourceAuto – The IF filter type is automatically chosen.

naIFFilterSourceManual – The IF filter is a predetermined shape where the IFFilterSampleCount determines the number of taps in the filter.

Return Type NAIFFilterSource

Default naIFFilterSourceAuto

Examples `App.ActiveChannel.IFConfiguration.IFFilterSource =
naIFFilterSourceManual 'Write`

`Variable = App.ActiveChannel.IFConfiguration.IFFilterSource 'Read`

[See an example program](#)

C++ Syntax HRESULT get_IFFilterSource(tagNAIFFilterSource * pFilterSource);
HRESULT put_IFFilterSource(tagNAIFFilterSource filterSource);

Interface IIFConfiguration2

IFGainLevel Property

Description Manually sets the gain level for the specified receiver.

VB Syntax *IfConfig*.IFGainLevel (*id*) = *value*

Variable **(Type) - Description**

IfConfig An [IFConfiguration](#) (**object**)

id Receiver for which to set the gain level. Choose from: 'A', 'B', 'R1', 'R2'.

Note: The A and R1 receivers are always switched together. B and R2 are also always switched together. For example, if you specify 'A', R1 will also be switched.

value (long Integer) Gain Level. Choose from:

0 - Lowest gain setting

1

2 - Highest gain setting

Return Type Long Integer

Default 0 (Lowest setting)

Examples `IfConfig.IFGainLevel('A') = 1`

C++ Syntax HRESULT get_IFGainLevel (BSTR IDString, *GainLevel)

HRESULT put_IFGainLevel (BSTR IDString, GainLevel)

Interface IFConfiguration

IFGainMode Property

Description Sets the gain state for ALL receivers to Auto or Manual.

VB Syntax *IfConfig*.IFGainMode (*id*) = *value*

Variable **(Type) - Description**

IfConfig An [IFConfiguration](#) (**object**)

id Receivers for which to set the state. Choose 'ALL'.

value **(enum as NAModes)**

Choose from:

0 - naAUTO

1 - naMANUAL (use [IFGainLevel Property](#) to manually set gain level)

Return Type NAModes

Default 0 - naAUTO

Examples `IfConfig.IFGainMode("ALL") = naAUTO`

C++ Syntax HRESULT get_IFGainMode (BSTR IDString, NAModes *gainMode)

HRESULT put_IFGainMode (BSTR IDString, NAModes gainMode)

Interface IIFConfiguration

IFGateEnable Property

Description Sets or retrieves the state of the IF Gate.

Note: An error will occur if this command is used on a PNA without option H08 installed.

VB Syntax *IfConfig*.IFGateEnable = *value*

Variable (Type) - Description

IfConfig IFConfiguration (object)

value **(Boolean)** – The state of the IF Gate.

True – The IF Gate is in use.

False – The IF Gate is not in use.

Return Type Boolean

Default False

Examples `App.ActiveChannel.IFConfiguration.IFGateEnable = True 'Write`

`variable = App.ActiveChannel.IFConfiguration.IFGateEnable 'Read`

[See an example program](#)

C++ Syntax HRESULT get_IFGateEnable(VARIANT_BOOL * pGateEnabled);

HRESULT put_IFGateEnable(VARIANT_BOOL gateEnabled);

Interface IIFConfiguration

IFNumerator Property

Description Sets or returns the numerator value of the IF Fractional Multiplier.
Only applies to 2 stage mixers!

VB Syntax *mixer*.IFNumerator = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

value **(Long)**

Return Type long

Default Not Applicable

Examples `Print mixer.IFNumerator` 'prints the value of the IFNumerator

C++ Syntax HRESULT get_IFNumerator(long *pVal)
HRESULT put_IFNumerator(long newVal)

Interface IMixer

IFSideband Property

Description Sets or returns the value of the IF sideband, high or low.
Only applies to 2 stage mixers!

VB Syntax *mixer.IFSideband =value*

Variable **(Type) - Description**

mixer A Mixer **(object)**

value **(enum as FCASideBand)** - Choose from:

0 - LOW

1 - HIGH

Return Type FCASideBand

Default 0 - LOW

Examples `Print mixer.IFSideband 'prints the value of the IFSideband`

C++ Syntax HRESULT get_IFSideband(FCASideBand *pVal)
HRESULT put_IFSideband(FCASideBand newVal)

Interface IMixer

IFSourcePath Property

Description Sets the source path of the specified receiver. An error is returned if *<id>* is not valid, or if *<value>* is not valid for the specified *<id>*.

VB Syntax *IfConfig*.IFSourcePath (*id*) = *value*

Variable **(Type) - Description**

IfConfig An [IFConfiguration](#) (object)

id Receiver for which to set the gain level. Choose from: 'A', 'B', 'R1', 'R2'..

Note: The A and R1 receivers are always switched together. B and R2 are also always switched together. For example, if you specify "A", R1 will also be switched.

value **(Enum as NAIFSourcePath)** Source path. Choose from:

0 - **naNormalIFPath** - the PNA decides the appropriate IF input paths.

1 - **naExternalIFPath** - always use the rear panel IF inputs.

Return Type NAIFSourcePath

Default 0 - naNormalIFPath

Examples `IfConfig.IFSourcePath('A') = naNormalIFPath`

C++ Syntax HRESULT get_IFSourcePath (BSTR IDString, naIFSourcePath *IFSourcePath)

HRESULT put_IFSourcePath (BSTR IDString, naIFSourcePath IFSourcePath)

Interface IIFConfiguration

IFStartFrequency Property

Description Sets or returns the start frequency value of the mixer IF frequency.

Only applies to 2 stage mixers!

VB Syntax *mixer*.IFStartFrequency = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

value **(double)** - Frequency in Hertz.

Return Type Double

Default Not Applicable

Examples `Print mixer.IFStartFrequency` 'prints the value of the
IFStartFrequency

C++ Syntax HRESULT get_IFStartFrequency(double *pVal)
HRESULT put_IFStartFrequency(double newVal)

Interface IMixer

IFStopFrequency Property

Description Sets or returns the stop frequency value of the mixer IF frequency.

Only applies to 2 stage mixers!

VB Syntax *mixer*.IFStopFrequency = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

value **(double)** - IF stop frequency in Hertz.

Return Type Double

Default Not Applicable

Examples `Print mixer.IFStopFrequency` 'prints the value of the
IFStopFrequency

C++ Syntax HRESULT get_IFStopFrequency(double *pVal)
HRESULT put_IFStopFrequency(double newVal)

Interface IMixer

Write/Read

ImpulseWidth Property

Description	Sets or returns the Impulse Width of Time Domain transform windows
VB Syntax	<i>trans.ImpulseWidth = value</i>
Variable	(Type) - Description
<i>trans</i>	A <u>Transform</u> (object)
<i>value</i>	(double) - Impulse Width in seconds. Range of settings depends on the frequency range of your analyzer.
Return Type	Double
Default	.98 / Default Span
Examples	<pre>trans.ImpulseWidth = 200e-12 'sets the Impulse width of a transform window -Write IW = trans.ImpulseWidth 'Read</pre>
C++ Syntax	HRESULT get_ImpulseWidth(double *pVal) HRESULT put_ImpulseWidth(double newVal)
Interface	ITransform

IndexState Property

Description Determines the control of Material Handler connector Pin 20.

VB Syntax *handler.IndexState = value*

Variable **(Type) - Description**

handler **(object)** - A Handler I/O object

value **(boolean)**
0 (False) - Pin 20 is controlled by Output Port B6
1(True) - Pin 20 is controlled by the Index signal

Return Type Boolean

Default

Examples `handler.IndexState = False 'Write
bState = handler.IndexState 'Read`

C++ Syntax HRESULT put_IndexState (BOOL *pVal);
HRESULT get_IndexState (BOOL newVal);

Interface IHWMaterialHandlerIO2

InputA Property - OBSOLETE

Description	This property has NO replacement and no longer works correctly. (Sept. 2004) Sets a Port Extension value for Receiver A
VB Syntax	<code>portExt.InputA = value</code>
Variable	(Type) - Description
<code>portExt</code>	A Port Extension (object)
<code>value</code>	(double) - Port Extension value in seconds. Choose any number between -10 and 10
Return Type	Double
Default	0
Examples	<pre>portExt.InputA = 10e-6 'Write inA = portExt.InputA 'Read</pre>
C++ Syntax	HRESULT get_InputA(double *pVal) HRESULT put_InputA(double newVal)
Interface	IPortExtension

Write/Read

InputB Property - OBSOLETE

Description	This property has NO replacement and no longer works correctly. (Sept. 2004) Sets the Port Extension value for Receiver B
VB Syntax	<code>portExt.InputB = value</code>
Variable	(Type) - Description
<code>portExt</code>	A Port Extension (object)
<code>value</code>	(double) - Port Extension value in seconds. Choose any number between -10 and 10
Return Type	Double
Default	0
Examples	<pre>portExt.InputB = 10e-6 'Write inB = portExt.InputB 'Read</pre>
C++ Syntax	HRESULT get_InputB(double *pVal) HRESULT put_InputB(double newVal)
Interface	IPortExtension

Write/Read

InputC Property OBSOLETE

Description **This property has NO replacement and no longer works correctly. (Sept. 2004)**

Sets the Port Extension value for Receiver C

VB Syntax `portExt.InputC = value`**Variable** **(Type) - Description**`portExt` A Port Extension (**object**)`value` (**double**) - Port Extension value in seconds. Choose any number between **-10** and **10****Return Type** Double**Default** 0**Examples** `portExt.InputC = 10e-6 'Write``inC = portExt.InputC 'Read`**C++ Syntax** HRESULT get_InputC(double *pVal)
HRESULT put_InputC(double newVal)**Interface** IPortExtension

InputDenominator Property

Description Sets or returns the denominator value of the Input Fractional Multiplier.

VB Syntax `mixer.InputDenominator = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(Long)** - Input denominator value.

Return Type Long

Default 1

Examples `Print mixer.InputDenominator 'prints the value of the InputDenominator`

C++ Syntax HRESULT get_InputDenominator(long *pVal)
HRESULT put_InputDenominator(long newVal)

Interface IMixer

IsInputGreaterThanLO Property

Description Specifies whether to use the Input frequency that is greater than the LO or less than the LO. To learn more, see the [mixer setup dialog box help](#).

VB Syntax `mixer.IsInputGreaterThanLO (LO) = bool`

Variable **(Type) - Description**

mixer A Mixer **(object)**

LO (Integer) - LO stage number
Choose from 1 (default) or 2

bool **(Boolean) -**

True (1) - Use the Input that is Greater than the specified LO.

False (0) - Use the Input that is Less than the specified LO.

Return Type Boolean

Default True

Examples `mixer.IsInputGreaterThanLO(1) = True`

C++ Syntax HRESULT get_IsInputGreaterThanLO(VARIANT_BOOL * val);
HRESULT put_IsInputGreaterThanLO(VARIANT_BOOL val);

Interface IMixer2

InputNumerator Property

Description Sets or returns the numerator value of the Input Fractional Multiplier.

VB Syntax `mixer.InputNumerator = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(Long)** - Input numerator value.

Return Type Long

Default 1

Examples `Print mixer.InputNumerator` 'prints the value of the InputNumerator

C++ Syntax HRESULT get_InputNumerator(long *pVal)
HRESULT put_InputNumerator(long newVal)

Interface IMixer

InputPower Property

Description Sets or returns the value of the Input Power.

VB Syntax `mixer.InputPower = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(double)** - Input power in dBm.

Return Type Double

Default -17dBm

Examples `Print mixer.InputPower 'prints the value of the InputPower`

C++ Syntax HRESULT get_InputPower(double *pVal)
HRESULT put_InputPower(double newVal)

Interface IMixer

InputStartFrequency Property

Description Sets and returns the start frequency value of the mixer Input frequency.

VB Syntax `mixer.InputStartFrequency = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(double)** - Input start frequency in Hertz.

Return Type Double

Default Start frequency of the PNA

Examples `mixer.InputStartFrequency = Start_Freq`

C++ Syntax HRESULT get_InputStartFrequency(double *pVal)
HRESULT put_InputStartFrequency(double newVal)

Interface IMixer

InputStopFrequency Property

Description Sets and returns the stop frequency value of the mixer Input frequency.

VB Syntax `mixer.InputStopFrequency = value`

Variable (Type) - Description

mixer A Mixer **(object)**

value **(double)** - Input stop frequency in Hertz.

Return Type Double

Default Stop frequency of the PNA

Examples `mixer.InputStopFrequency = Stop_Freq`

C++ Syntax HRESULT get_InputStopFrequency(double *pVal)
HRESULT put_InputStopFrequency(double newVal)

Interface IMixer

InternalTestsetPortCount Property

Description Returns the number of PNA test ports on the internal testset.

VB Syntax `value = cap.InternalTestsetPortCount`

Variable **(Type) - Description**

`value` (Long) - Variable to store the returned number of PNA test ports.

`cap` A [Capabilities](#) (object)

Return Type Long

Default Not Applicable

Examples `value = cap.InternalTestsetPortCount 'Read`

C++ Syntax HRESULT get_InternalTestsetPortCount(long * numPorts);

Interface ICapabilities

Interpolate Correction Property

Description Turns ON and OFF correction interpolation which calculates new error terms when stimulus values change after calibration.

When this property is ON and error correction is being applied, the calibration subsystem attempts to interpolate the error terms whenever the stimulus parameters are changed.

When this property is OFF under the same circumstances, error correction is turned OFF.

VB Syntax `meas.InterpolateCorrection = value`

Variable (Type) - Description

`meas` A Measurement (**object**)

`value` (**boolean**) - Choose from:

True - Turns correction interpolation ON

False - Turns correction interpolation OFF

Return Type Boolean

Default True

Examples `meas.InterpolateCorrection = False`

`calInterpolate = InterpolateCorrection 'Read`

C++ Syntax HRESULT get_InterpolateCorrection(boolean *pVal)
HRESULT put_InterpolateCorrection(boolean newVal)

Interface IMeasurement

Interrupt Property

Description	Reads the boolean that represents the state of the Interrupt In line (pin 13) on the external test set connector.
VB Syntax	<code>value = ExtIO.Interrupt</code>
Variable	(Type) - Description
<i>value</i>	(boolean) - Variable to store the returned data
<i>ExtIO</i>	(object) - An ExternalTestSetIO object
Return Type	Boolean False (0) - indicates the line is being held at a TTL High True (1) - indicates the line is being held at a TTL Low
Default	Not Applicable
Examples	<code>value = ExtIO.Interrupt</code>
C++ Syntax	<code>HRESULT get_Interrupt(VARIANT_BOOL* bValue);</code>
Interface	IHWExternalTestSetIO

IsContinuous Property

Description Returns whether or not a channel is in continuous mode. To set the channel to continuous mode, use [Continuous Method](#).

VB Syntax *value* = *chan*.IsContinuous

Variable (Type) - Description

value **(boolean)** - Choose either:

False (0) - Channel trigger is NOT set to continuous.

True (1) - Channel trigger IS set to continuous.

chan Channel **(object)**

Return Type boolean

Default Not Applicable

Examples `trig = chan.IsContinuous 'Read`

C++ Syntax HRESULT get_IsContinuous (VARIANT_BOOL *bContinuous);

Interface IChannel3

IsECALModuleFoundEx Property

Description	This property replaces IsECALModuleFound Property . Returns true or false depending on whether communication was established between the PNA and the specified ECal module.
VB Syntax	<i>modFound</i> = <i>cal</i> .IsECALModuleFoundEx (<i>module</i>)
Variable	(Type) - Description
<i>modFound</i>	(boolean) - Variable to store the returned test result. True - The PNA identified the presence of the specified ECal module. False - The PNA did NOT identify the presence of the specified ECal module.
<i>cal</i>	(object) - A Calibrator object
<i>module</i>	(long integer) ECal module. Choose from modules 1 through 8 Use GetECALModuleInfoEx to return the model and serial number of each module.
Return Type	Boolean
Default	Not applicable
Examples	<pre>Set cal = pna.ActiveChannel.Calibrator moduleFound = cal.IsECALModuleFoundEx(1)</pre>
C++ Syntax	HRESULT get_IsECALModuleFoundEx(long moduleNumber, VARIANT_BOOL *bModuleFound);
Interface	ICalibrator4

IsFrequencyOffsetPresent Property

Description	Returns a value indicating the presence of Frequency Offset Option 080 in the remote PNA.
VB Syntax	<i>value</i> = <i>cap</i> .IsFrequencyOffsetPresent
Variable	(Type) - Description
<i>value</i>	(Boolean) - Variable to store the returned value (True or False).
<i>cap</i>	A Capabilities (object)
Return Type	Boolean
Default	Not Applicable
Examples	<pre>value = cap.isFrequencyOffsetPresent(1) 'Read</pre>
C++ Syntax	HRESULT get_IsFrequencyOffsetPresent(VARIANT_BOOL * present);
Interface	ICapabilities

IsHold Property

Description	Returns whether or not a channel is in hold mode. To set the channel to hold mode, use Hold Method .
VB Syntax	<i>value</i> = <i>chan</i> .IsHold
Variable	(Type) - Description
<i>value</i>	(boolean) - Choose either: False (0) - Channel trigger is NOT set to hold. True (1) - Channel trigger IS set to hold.
<i>chan</i>	Channel (object)
Return Type	boolean
Default	Not Applicable
Examples	<pre>trig = chan.IsHold 'Read</pre>
C++ Syntax	HRESULT get_IsHold (VARIANT_BOOL *bHold);
Interface	IChannel3

IsReceiverStepAttenuatorPresent Property

Description Returns a value indicating the presence of Receiver step attenuators in the remote PNA.

VB Syntax `value = cap.IsReceiverStepAttenuatorPresent (n)`

Variable (Type) - Description

`value` **(Boolean)** - Variable to store the returned value.

`cap` A Capabilities **(object)**

`n` **(Long)** - port number to query for step attenuators

Return Type Boolean

Default Not Applicable

Examples `value = cap.IsReceiverStepAttenuatorPresent(1) 'Read`

C++ Syntax HRESULT get_IsReceiverStepAttenuatorPresent(long portNumber, VARIANT_BOOL * present);

Interface ICapabilities

IsReferenceBypassSwitchPresent Property

Description	Returns a value indicating the presence of a Reference Bypass Switch in the remote PNA.
VB Syntax	<i>value</i> = <i>cap</i> .IsReferenceBypassSwitchPresent (<i>n</i>)
Variable	(Type) - Description
<i>value</i>	(Boolean) - Variable to store the returned value (True or False).
<i>cap</i>	A <u>Capabilities</u> (object)
<i>n</i>	(Long) - port number to query for reference bypass switch
Return Type	Boolean
Default	Not Applicable
Examples	<pre>value = cap.IsReferenceBypassSwitchPresent(1) 'Read</pre>
C++ Syntax	HRESULT get_IsReferenceBypassSwitchPresent(long portNumber, VARIANT_BOOL * present);
Interface	ICapabilities

Read-only

IsSParameter Property

Description Returns true if measurement represents an S-Parameter

VB Syntax *value* = *meas*.IsSparameter

Variable (Type) - Description

meas A Measurement (**object**)

value (**Boolean**)

1 True - measurement is an S-Parameter

0 False - measurement is NOT an S-Parameter

Return Type Boolean

Default True

Examples `print app.IsSparameter`

C++ Syntax HRESULT IsSparameter([out, retval] VARIANT_BOOL * bVal);

Interface IMeasurement2

IterationsTolerance Property

Description Sets the maximum desired deviation from the sum of the test port power and the offset value. Power readings will continue to be made, and source power adjusted, until a reading is within this tolerance value or the max number of readings has been met. The last value to be read is the valid reading for that data point.

VB Syntax *pwrCal.IterationsTolerance = value*

Variable (Type) - Description

pwrCal **(object)** - A SourcePowerCalibrator (object)

value **(Double)** – Tolerance value in dBm. Choose any number between 0 and 5

Return Type Double

Default .05 dB

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.IterationsTolerance = .1 'Write
ReadTol = powerCalibrator.IterationsTolerance 'Read
```

C++ Syntax HRESULT get_IterationsTolerance(double *pVal);
HRESULT put_IterationsTolerance(double newVal);

Interface ISourcePowerCalibrator3

Write/Read

KaiserBeta Property

Description Sets or returns the Kaiser Beta of Time Domain transform windows**VB Syntax** *trans.KaiserBeta = value***Variable** (Type) - Description*trans* A Transform (**object**)*value* (**single**) - Kaiser Beta. Choose any number between **0** and **13**.**Return Type** Single**Default** 0**Examples**

```
trans.KaiserBeta = 6 'sets the Kaiser Beta of a transform window
-Write
```

```
KB = trans.KaiserBeta 'Read
```

C++ Syntax HRESULT get_KaiserBeta(float *pVal)
HRESULT put_KaiserBeta(float newVal)**Interface** ITransform

L0 Property

Description Sets and Returns the L0 (L-zero) value (the first inductance value) for the calibration standard.

To set the other inductance values, use [L1](#), [L2](#), [L3](#)

VB Syntax `calstd.L0 = value`

Variable **(Type) - Description**

`calstd` A CalStandard **(object)**. Use `calKit.GetCalStandard` to get a handle to the standard.

`value` **(single)** - Value for L0 in picohenries

Return Type Single

Default Not Applicable

Examples `calstd.L0 = 15 'Write the value of L0 = 15picohenries`

`Induct0 = calstd.L0 'Read the value of L0`

C++ Syntax `HRESULT get_L0(float *pVal)`
`HRESULT put_L0(float newVal)`

Interface ICalStandard

Write/Read

L1 Property

Description Sets and Returns the L1 value (the second inductance value) for the calibration standard.
To set the other inductance values, use [L0](#), [L2](#), [L3](#)

VB Syntax `calstd.L1 = value`

Variable **(Type) - Description**

`calstd` A CalStandard **(object)**. Use calKit.[GetCalStandard](#) to get a handle to the standard.

`value` **(single)** - Value for L1 in picohenries

Return Type Single

Default Not Applicable

Examples `calstd.L1 = 15 'Write the value of L1 = 15picohenries`

`Induct1 = calstd.L1 'Read the value of L1`

C++ Syntax HRESULT get_L1(float *pVal)
HRESULT put_L1(float newVal)

Interface ICalStandard

Write/Read

L2 Property

Description Sets and Returns the L2 value (the third inductance value) for the calibration standard.
To set the other inductance values, use [L0](#), [L1](#), [L3](#)

VB Syntax `calstd.L2 = value`

Variable **(Type) - Description**

`calstd` A CalStandard **(object)**. Use `calKit.GetCalStandard` to get a handle to the standard.

`value` **(single)** - Value for L2 in picohenries

Return Type Single

Default Not Applicable

Examples `calstd.L2 = 15 'Write the value of L2 to 15picohenries`

`Induct2 = calstd.L2 'Read the value of L2`

C++ Syntax HRESULT get_L2(float *pVal)
HRESULT put_L2(float newVal)

Interface ICalStandard

Write/Read

L3 Property

Description Sets and Returns the L3 value (the third inductance value) for the calibration standard.
To set the other inductance values, use [L0](#), [L1](#), [L2](#)

VB Syntax `calstd.L3 = value`

Variable **(Type) - Description**

`calstd` A CalStandard **(object)**. Use `calKit.GetCalStandard` to get a handle to the standard.

`value` **(single)** - Value for L3 in picohenries

Return Type Single

Default Not Applicable

Examples `calstd.L3 = 15 'Write the value of L3 to 15picohenries`

`Induct3 = calstd.L3 'Read the value of L3`

C++ Syntax HRESULT get_L3(float *pVal)
HRESULT put_L3(float newVal)

Interface ICalStandard

Write/Read

Label Property

Description Sets and Returns the label for the calibration standard. The label is used to prompt the user to connect the specified standard.

VB Syntax `calstd.Label = value`

Variable (Type) - Description

calstd A CalStandard (**object**). Use `calKit.GetCalStandard` to get a handle to the standard.

value (**string**) - between 1 and 12 characters long. Cannot begin with a numeric.

Return Type String

Default Not Applicable

Examples `calstd.Label = "Short" 'Write`

`stdLabel = calstd.Label 'Read`

C++ Syntax HRESULT get_Label(BSTR *pVal)
HRESULT put_Label(BSTR newVal)

Interface ICalStandard

LastModified Property

Description Returns the time stamp of the last modification to this CalSet

VB Syntax *value* = *Object*.**LastModified**

Variable (Type) - Description

object Channel **(object)**

or

CalSet **(object)** - Read-only property

value **(Variant)** – Variable to store the time stamp.

Return Type Variant

Default Not Applicable

Examples `date = CalSet.LastModified 'Read`

C++ Syntax HRESULT get_LastModified(VARIANT* datetime)

Interface ICalSet3

Read-only

LimitTestFailed Property

Description Returns the results of limit testing for the measurement.

VB Syntax `testFailed = meas.LimitTestFailed`

Variable **(Type) - Description**

testFailed **(boolean)** Variable to store the returned value

False (0) - Limit Test Passed

True (1) - Limit Test Failed

meas A Measurement **(object)**

Return Type Boolean

Default False returned if there is no testing in progress

Examples

```
Dim testRes As Boolean
testRes = meas.LimitTestFailed
MsgBox (testRes)
```

C++ Syntax HRESULT get_LimitTestFailed(VARIANT_BOOL*
truelFailed)

Interface IMeasurement

Write/Read

EndStimulus Property

Description When constructing a limit line, specifies the stimulus value for the end of the segment.**VB Syntax** *limtseg.EndStimulus = value***Variable** **(Type) - Description***limtseg* A LimitSegment (**object**)*value* (**double**) - End Stimulus X-axis value. No units**Return Type** Double**Default** 0

Examples

```
Set limtseg = meas.LimitTest(1)
limtseg.EndStimulus = 8e9 'Write

EndStim = limtseg.EndStimulus 'Read
```

C++ Syntax HRESULT get_EndStimulus(double *pVal)
 HRESULT put_EndStimulus(double newVal)

Interface ILimitSegment

Write/Read

EndResponse Property

Description When constructing a limit line, specifies the amplitude value at the end of the limit segment.**VB Syntax** *limtseg.EndResponse* = *value***Variable (Type) - Description***limts* A LimitSegment (**object**)*value* (**double**) - Y-axis value of the End Response limit. No units**Return Type** Double**Default** 0

Examples

```
Set limtseg = meas.LimitTest(1)
limtseg.EndResponse = 10 'Write

EndResp = limtseg.EndResponse 'Read
```

C++ Syntax HRESULT get_EndResponse(double *pVal)
 HRESULT put_EndResponse(double newVal)

Interface ILimitSegment

Write/Read

Type (limit) Property

Description Specifies the Limit Line type.**VB Syntax** `limt(index).Type = value`**Variable (Type) - Description***limt* A LimitSegment (**object**)*index* (**variant**) - Limit line number in the LimitTest collection

value (**enum NALimitSegmentType**) - Limit Line type. Choose from:
0 - naLimitSegmentType_OFF - turns limit line OFF
1 - naLimitSegmentType_Maximum - limit line fails with a data point ABOVE the line
2 - naLimitSegmentType_Minimum - limit line fails with a data point BELOW the line

Return Type Long Integer**Default** 0 - OFF**Examples**

```
Set limts = meas.LimitTest
limts.Type = naLimitSegmentType_Maximum 'Write
```

```
limitType = limts.Type 'Read
```

C++ Syntax HRESULT put_Type(tagNALimitSegmentType *pVal)
 HRESULT get_Type(tagNALimitSegmentType newVal)

Interface ILimitSegment

LineDisplay Property

Description Turns the display of limit lines ON or OFF. To turn limit TESTING On and OFF, use [State Property](#).

Note: Trace data must be ON to view limit lines

VB Syntax `limitst.LineDisplay = state`

Variable (Type) - Description

`limitst` A LimitTest (**object**)

`state` (**boolean**)
0 - Turns the display of limit lines OFF
1 - Turns the display of limit lines ON

Return Type Long Integer

Default 1 - ON

Examples `Limtttest.LineDisplay = 1 'Write`

`lineDsp = Limtttest.LineDisplay 'Read`

C++ Syntax HRESULT get_LineDisplay(VARIANT_BOOL *pVal)
HRESULT put_LineDisplay(VARIANT_BOOL newVal)

Interface ILimitTest

LoadCharFromFile Property

Description Sets and returns whether a Mixer characterization file is to be loaded. Specify and load the filename with CharFileName Property

VB Syntax `VMC.LoadCharFromFile = bool`

Variable **(Type) - Description**

VMC VMCType (object)

bool (Boolean)

1 - Load from file

0 - Perform mixer characterization

Return Type Boolean

Default 0

Examples `value = VMC.LoadCharFromFile`

C++ Syntax `HRESULT put_LoadCharFromFile(VARIANT_BOOL bLoadCharFromFile);`
`HRESULT get_LoadCharFromFile(VARIANT_BOOL *bLoadCharFromFile);`

Interface VMCType

Read-only

LoadPort Property

Description Returns the load port number associated with an S-parameter reflection measurement. If the measurement is not a reflection S-parameter, the number returned by this property will have no meaning.

VB Syntax `loadPort = meas.LoadPort`

Variable (Type) - Description

`loadPort` **(long integer)** - The reflection measurement's load port number.

`meas` A Measurement **(object)**

Return Type Long Integer

Default Not Applicable

Examples

```
Set meas = pna.ActiveMeasurement
loadPort = meas.LoadPort
```

C++ Syntax HRESULT get_LoadPort(long *pPortNumber);

Interface IMeasurement

Write/Read

LocalLockoutState Property

Description Prevents use of the mouse, keyboard, and front panel while your program is running. Use of these controls while this property is set TRUE causes an error message on the PNA display. To prevent these messages, see [About Error Messages](#).

VB Syntax `app.LocalLockoutState = bool`

Variable **(Type) - Description**

app An [Application](#) (**object**)

bool (**boolean**) -Choose either:

0 (False) - User Interface is NOT locked out.

1 (True) - User Interface IS locked out.

Return Type Boolean

Default 0 - False

Examples `app.LocalLockoutState = True 'Write`

```
block = app.LocalLockoutState 'Read
```

C++ Syntax HRESULT get_LocalLockoutState(VARIANT_BOOL *State);
HRESULT put_LocalLockoutState(VARIANT_BOOL *State);

Interface IApplication4

LODenominator Property

Description Sets or returns the denominator value of the LO Fractional Multiplier.

VB Syntax `mixer.LODenominator (n) = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(Long)** - LO denominator value

`n` **(Long)** - LO stage number

Choose from 1 or 2

Return Type Long

Default 1

Examples `Print mixer.LODenominator(1) 'prints the value of the first LODenominator`

C++ Syntax HRESULT get_LODenominator(long *pVal)
HRESULT put_LODenominator(long newVal)

Interface IMixer

LOFixedFrequency Property

Description Sets or returns the LO frequency value

VB Syntax `mixer.LOFixedFrequency (n) = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(double)** - LO Frequency in Hertz.

`n` **(Long)** - LO stage number

Choose from 1 or 2

Return Type Double

Default 0 Hz

Examples `Print mixer.LOFixedFrequency(1) 'prints the value of the first
LO fixed frequency`

C++ Syntax HRESULT get_LOFixedFrequency(double *pVal)

HRESULT put_LOFixedFrequency(double newVal)

Interface IMixer

LOName Property

Description Sets or returns the name of the external LO source.

VB Syntax *mixer.LOName (n) =value*

Variable (Type) - Description

mixer A Mixer **(object)**

n **(Long)** - LO stage number

Choose from 1 or 2

value **(string)** - External LO Source name. Must be a valid source name already configured on the PNA. The source must also be connected properly..

Return Type String

Default "Not controlled"

Examples `mixer.LOName(1) = "MySource"`

C++ Syntax HRESULT get_LOName(string *pVal)
HRESULT put_LOName(string newVal)

Interface MIXer

LONumerator Property

Description Sets or returns the numerator value of the LO Fractional Multiplier.

VB Syntax *mixer.LONumerator* (*n*) = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

value **(Long)** - LO denominator value

n **(Long)** - LO stage number

Choose from 1 or 2

Return Type Long

Default 1

Examples `Print mixer.LONumerator(1) 'prints the value of the
first LO Numerator`

C++ Syntax HRESULT get_LONumerator(long *pVal)
HRESULT put_LONumerator(long newVal)

Interface IMixer

LOPower Property

Description Sets or returns the value of LO Power.

VB Syntax *mixer.LOPower (n) = value*

Variable (Type) - Description

mixer A Mixer **(object)**

n **(Long)** - LO stage number
Choose from 1 or 2

value **(double)** - LO Power in dBm.

Return Type Double

Default -10dBm

Examples `Print mixer.LOPower(1) 'prints the value of the LO Power`

C++ Syntax HRESULT get_LOPower(double *pVal)
HRESULT put_LOPower(double newVal)

Interface IMixer

LORangeMode Property

Description Sets or returns the LO sweep mode.

VB Syntax *mixer.LORangeMode* (*n*) = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

n **(Long)** - LO stage number.

Choose from 1 or 2

value **(Enum as MixerRangeMode)** - LO sweep mode. Choose from:

0 - **mixSwept**

1 - **mixFixed**

Return Type Enum

Default 0 - mixSwept

Examples `mixer.LORangeMode(1)=mixSwept`

C++ Syntax HRESULT get_LORangeMode(long *pVal)

HRESULT put_LORangeMode(long newVal)

Interface IMixer3

Loss Property

Description Sets and Returns the insertion loss for the calibration standard.

VB Syntax `calstd.loss = value`

Variable (Type) - Description

`calstd` A CalStandard **(object)**. Use calKit.[GetCalStandard](#) to get a handle to the standard.

`value` **(single)** - Insertion loss in Mohms / sec. (MegaOhms per second of electrical delay)

Return Type Single

Default Not Applicable

Examples `calstd.loss = 3.5e9 'Write`

`stdLoss = calstd.loss 'Read the value of Loss`

C++ Syntax HRESULT get_Loss(float *pVal)
HRESULT put_Loss(float newVal)

Interface ICalStandard

Loss (Source Power Cal) Property

Description Sets or returns the loss value associated with a PowerLossSegment.

VB Syntax *lossSeg.Loss = value*

Variable (Type) - Description

lossSeg **(object)** - PowerLossSegment

value **(double)** – Loss value in dB. This can be any value between 0 and 200.

Return Type Double

Default 0

Examples `lossSeg.Loss = 0.5 'Write`
`lossVal = lossSeg.Loss 'Read`

C++ Syntax HRESULT put_Loss(Double newVal);
HRESULT get_Loss(Double *pVal);

Interface IPowerLossSegment

LOStage Property

Description Sets or returns the number of LO stages present in the mixer.

VB Syntax `mixer.LOStage = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(Long)** - Number of LO stages. Choose from **1** or **2**

Return Type Long

Default 1

Examples `mixer.LOStage = 1 'sets the LO Stage value to 1`

C++ Syntax HRESULT get_LOStage(long *pVal)
HRESULT put_LOStage(long newVal)

Interface IMixer

LOStartFrequency Property

Description Sets or returns the LO start frequency value. This command can only be used with SMC (not VMC) measurements.

VB Syntax `mixer.LOStartFrequency (n) = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(double)** - LO Start Frequency in Hertz.

`n` **(Long)** - LO stage number
Choose from 1 or 2

Return Type Double

Default

Examples `Print mixer.LOStartFrequency(1) 'prints the value of the first LO start frequency`

C++ Syntax HRESULT get_LOStartFrequency(long id, double *pVal)
HRESULT put_LOStartFrequency(long id, double newVal)

Interface IMixer3

LOStopFrequency Property

Description Sets or returns the LO stop frequency value. This command can only be used with SMC (not VMC) measurements.

VB Syntax `mixer.LOStopFrequency (n) = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(double)** - LO Stop Frequency in Hertz.

`n` **(Long)** - LO stage number
Choose from 1 or 2

Return Type Double

Default

Examples `Print mixer.LOStopFrequency(1)` 'prints the value of the first LO stop frequency

C++ Syntax HRESULT get_LOStopFrequency(long id, double *pVal)
HRESULT put_LOStopFrequency(long id, double newVal)

Interface IMixer3

MagnitudeOffset Property

Description Offsets the data trace magnitude by the specified value.
To offset the data trace magnitude to a slope value that changes with frequency, use [MagnitudeSlopeOffset Property](#).
To implement a Receiver Cal offset, use [LogMagnitudeOffset property](#).

VB Syntax `meas.MagnitudeOffset = value`

Variable **(Type) - Description**

`meas` **(object)** - A [Measurement](#) object

`value` **(double)** - Offset value in dB.

Return Type Double

Default 0

Examples `meas.MagnitudeOffset = 4 'Write`

`offs = meas.MagnitudeOffset 'Read`

C++ Syntax HRESULT put_MagnitudeOffset(double newVal);
HRESULT get_MagnitudeOffset(double *pVal);

Interface IMeasurement4

MagnitudeSlopeOffset Property

Description Offsets the data trace magnitude to a value that changes linearly with frequency. The offset slope begins at 0 Hz.

To offset the entire data trace magnitude by a specified value, use [MagnitudeOffset Property](#).

VB Syntax `meas.MagnitudeSlopeOffset = value`

Variable **(Type) - Description**

`meas` **(object)** - A [Measurement](#) object

`value` **(double)** - Offset slope value in dB / 1GHz.

Return Type Double

Default 0

Examples `meas.MagnitudeSlopeOffset = 4 'Writes a slope offset of 4dB/1GHz.`

`offs = meas.MagnitudeSlopeOffset 'Read`

C++ Syntax HRESULT put_MagnitudeSlopeOffset(double newVal);
HRESULT get_MagnitudeSlopeOffset(double *pVal);

Interface IMeasurement4

Write/Read

MarkerFormat Property

Description Sets (or returns) the format of all the markers in the measurement. To override this setting for an individual marker, use **mark.Format**

VB Syntax `meas.MarkerFormat = value`

Variable (Type) - Description

`meas` A Measurement (**object**)

`value` (**enum NAMarkerFormat**) - Choose from:

- 0** - naMarkerFormat_LinMag
- 1** - naMarkerFormat_LogMag
- 2** - naMarkerFormat_Phase
- 3** - naMarkerFormat_Delay
- 4** - naMarkerFormat_Real
- 5** - naMarkerFormat_Imaginary
- 6** - naMarkerFormat_SWR
- 7** - naMarkerFormat_LinMagPhase
- 8** - naMarkerFormat_LogMagPhase
- 9** - naMarkerFormat_ReallImaginary
- 10** - naMarkerFormat_ComplexImpedance
- 11** - naMarkerFormat_ComplexAdmittance

Return Type Long Integer

Default 1 - naMarkerFormat_LogMag

Examples `meas.MarkerFormat = naMarkerFormat_SWR 'Write`

`fmt = mark.Format 'Read`

C++ Syntax HRESULT put_MarkerFormat(tagNAMarkerFormat NewFormat)

Interface IMeasurement

InterpolateMarkers Method

Description Turns **All** Marker Interpolation ON and OFF for the measurement. Marker interpolation enables X-axis resolution between the discrete data values. The analyzer will calculate the x and y-axis data values between discrete data points. To override this property for individual markers, use the [Interpolated](#) property.

VB Syntax `meas.Interpolate = value`

Variable **(Type) - Description**

meas A Measurement (**object**)

value (**boolean**)
False - Turns interpolation OFF for all markers in the measurement
True - Turns interpolation ON for all markers in the measurement

Return Type Boolean

Default True (ON)

Examples `meas.Interpolate = 1`

C++ Syntax HRESULT InterpolateMarkers(VARIANT_BOOL bNewVal)

Interface IMeasurement

Interpolated Property

Description Turns marker Interpolation ON and OFF. Marker interpolation enables X-axis resolution beyond the discrete data values. The analyzer will calculate the x and y-axis data values between discrete data points. Use `meas.Interpolate` to change interpolation of **all** markers in a measurement. This command will override the measurement setting.

VB Syntax `mark.Interpolated = value`

Variable **(Type) - Description**

`mark` A Marker (**object**)

`value` (**boolean**)
False - Turns interpolation OFF
True - Turns interpolation ON

Return Type Boolean

Default True (ON)

Examples `mark.Interpolated = 1 'Write`

`interpolate = mark.Interpolated 'Read`

C++ Syntax HRESULT `get_Interpolated(VARIANT_BOOL *pVal)`
HRESULT `put_Interpolated(VARIANT_BOOL newVal)`

Interface IMarker

Number Property

Description	Returns the number of the marker.
VB Syntax	<i>marknum</i> = <i>mark</i> . Number
Variable	(Type) - Description
<i>marknum</i>	(long) - Variable to store marker number
<i>mark</i>	A Marker (object)
Return Type	Long Integer
Default	Not applicable
Examples	<code>marknum = mark.Number 'Read</code>
C++ Syntax	HRESULT get_Number(long *pVal)
Interface	IMarker

MarkerReadout Property

Description	Enables or disables the readout of markers in the window. To show the marker on the screen use ShowMarkerReadout Method.
VB Syntax	<i>win</i> . MarkerReadout = <i>state</i>
Variable	(Type) - Description
<i>win</i>	A NAWindow (object)
<i>state</i>	(boolean) True (1) - enables marker readout False (0) - disables marker readout
Return Type	Boolean
Default	True
Examples	<pre>win.MarkerReadout = True 'Write State = app.ActiveNAWindow.MarkerReadout 'Read</pre>
C++ Syntax	HRESULT get_MarkerReadout(VARIANT_BOOL *pVal) HRESULT put_MarkerReadout(VARIANT_BOOL newVal)
Interface	INAWindow

MarkerReadoutSize Property

Description	Specifies the size of font used when displaying Marker Readout in the selected window.
VB Syntax	<i>win</i> . MarkerReadoutSize = <i>value</i>
Variable	(Type) - Description
<i>win</i>	A NAWindow (object)
<i>value</i>	(enum NAFontSize) 0 - naDefault - marker readout appears in default font size 1 - naLarge - marker readout appears in large font size
Return Type	Long Integer
Default	naDefault
Examples	<pre>win.MarkerReadoutSize = naDefault 'write default size for marker readout</pre> <pre>Dim Size As NAFontSize Size = app.ActiveNAWindow.MarkerReadoutSize 'Read</pre>
C++ Syntax	HRESULT get_MarkerReadoutSize(tagNAFontSize *pVal) HRESULT put_MarkerReadoutSize(tagNAFontSize newVal)
Interface	INAWindow

MarkerState Property

Description Sets or returns the ON / OFF state of the specified marker.

VB Syntax `meas.MarkerState (n) = state`

Variable (Type) - Description

`meas` A Measurement (**object**)

`n` (Long Integer) Marker number to turn on or off.

`state` (boolean) -
ON (1) turns the specified marker ON
OFF (0) turns the specified marker OFF

Return Type Boolean

Default 0 - OFF

Examples `meas.MarkerState(1) = True`

`reference = meas.MarkerState(2)`

C++ Syntax HRESULT get_MarkerState(long markerNum, VARIANT_BOOL bState)
HRESULT put_MarkerState(long markerNum, VARIANT_BOOL* bState)

Interface IMeasurement3

Write/Read

Type (Marker) Property

Description Sets and reads the marker type.**VB Syntax** `mark.Type = value`**Variable (Type) - Description***chan* A Marker (**object**)*value* (**enum NAMarkerType**) - Marker Type. Choose from:**0 - naMarkerType_Normal** - the X-axis value for a normal marker will always be determined by the measurement data of the marker.**1 - naMarkerType_Fixed** - retains and keeps its x-axis value at the time the marker type is set.**Return Type** Long Integer**Default** naMarkerType_Normal**Examples** `mark.Type = naMarkerType_Normal 'Write``MrkType = mark.Type 'Read`**C++ Syntax** HRESULT get_Type(tagNAMarkerType *pVal)
HRESULT put_Type(tagNAMarkerType newVal)**Interface** IMarker

Stimulus Property

Description Sets and reads the X-Axis value of the marker. If the marker is a delta marker, the value will be relative to the reference marker.

VB Syntax `mark.Stimulus = value`

Variable (Type) - Description

`mark` A Marker **(object)**

`value` **(double)** - X-Axis value. Choose any number within the full span of the channel or User Range (if set).

Return Type Double

Default First activated Marker turns ON in the middle of the X-axis range. Subsequent markers turn ON at the position of the most recently active marker.

Examples `mark.Stimulus = 3e9 'Write`

`XVal = mark.Stimulus 'Read`

C++ Syntax HRESULT get_Stimulus(double *pVal)
HRESULT put_Stimulus(double newVal)

Interface IMarker

Value Property

Description	<p>Reads the Y-Axis value of the marker. If the marker is a delta marker, the value will be relative to the reference marker.</p> <p>You cannot set the Y-axis value of a marker. The marker remains at the position at the time you set marker.Type.</p>
VB Syntax	<i>YValue</i> = <i>mark.Value</i> (<i>format</i>)
Variable	(Type) - Description
<i>YValue</i>	A variable to store the Y-axis value
<i>mark</i>	A Marker (object)
<i>format</i>	<p>(enum NAMarkerFormat) - The format you would like the marker's Y-axis value. The number in parenthesis following the format is the number of values that are returned in a variant array. Choose from:</p> <ul style="list-style-type: none"> 0 - naMarkerFormat_LinMag (1) 1 - naMarkerFormat_LogMag (1) 2 - naMarkerFormat_Phase (1) 3 - naMarkerFormat_Delay (1) 4 - naMarkerFormat_Real (1) 5 - naMarkerFormat_Imaginary (1) 6 - naMarkerFormat_SWR (1) 7 - naMarkerFormat_LinMagPhase (2) 8 - naMarkerFormat_LogMagPhase (2) 9 - naMarkerFormat_Reallmaginary (2) 10 - naMarkerFormat_ComplexImpedance (3) 11 - naMarkerFormat_ComplexAdmittance (3)
Return Type	Variant - The previous list of formats indicates the number of values that are returned in a variant array
Default	Not applicable
Examples	<pre>YVal = mark.Value 'Read</pre>
C++ Syntax	HRESULT get_Value(tagNAMarkerFormat format, VARIANT *pVal)
Interface	IMarker

MaximumFrequency Property

Description Sets and Returns the maximum frequency for the calibration standard.

VB Syntax `calstd.MaximumFrequency = value`

Variable (Type) - Description

calstd A CalStandard **(object)**. Use calKit.[GetCalStandard](#) to get a handle to the standard.

value **(double)** - Maximum frequency in Hertz.

Return Type Double

Default Not Applicable

Examples `calstd.MaximumFrequency = 9e9 'Write`

`maxFrequency = calstd.MaximumFrequency 'Read`

C++ Syntax HRESULT get_MaximumFrequency(double *pVal)
HRESULT put_MaximumFrequency(double newVal)

Interface ICalStandard

MaximumFrequency Property

Description Returns the maximum frequency of the remote PNA.

VB Syntax *value* = *cap*.MaximumFrequency

Variable (Type) - Description

value (Double) - Variable to store the returned maximum frequency of the PNA.

cap A Capabilities (**object**)

Return Type Double

Default Not Applicable

Examples `value = cap.MaximumFrequency 'Read`

C++ Syntax HRESULT get_MaximumFrequency(&frequencyMax);

Interface ICapabilities

MaximumFrequency (Source Power Cal) Property

Description Maximum usable frequency specified for the power sensor.

VB Syntax *pwrSensor*.MaximumFrequency = *value*

Variable (Type) - Description

pwrSensor **(object)** - A PowerSensor (object)

value **(double)** -Frequency in Hertz.

Return Type Double

Default 0

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.PowerSensors(1).MaximumFrequency = 6e9
'Write

MaxFreq = powerCalibrator.PowerSensors(1).MaximumFrequency
'Read
```

C++ Syntax HRESULT put_MaximumFrequency(double newVal);
HRESULT get_MaximumFrequency(double *pVal);

Interface IPowerSensor

MaximumIFFilterSampleCount Property

Description Returns the maximum allowed value for the [IFFilterSampleCount](#) property for the queried PNA.

Note: An error will occur if this command is used on a PNA without option H08 installed.

VB Syntax *IfConfig.MaximumIFFilterSampleCount = value*

Variable **(Type) - Description**

IfConfig [IFConfiguration](#) (object)

value **(long)** The maximum allowed value that can be applied to the [IFFilterSampleCount](#) property.

Return Type Long Integer

Default PNA Model number dependent

Examples

```
variable =
App.ActiveChannel.IFConfiguration.MaximumIFFilterSampleCount
'Read
```

[See an example program](#)

C++ Syntax HRESULT get_MaximumIFFilterSampleCount(long * pMaxSampleCount);

Interface IIFConfiguration2

MaximumIterationsPerPoint Property

Description Sets the maximum number of readings to take at each data point for iterating the source power. Power readings will continue to be made, and source power adjusted, until a reading is within the IterationsTolerance value or this max number of readings has been met. The last value to be read is the valid reading for that data point.

VB Syntax *pwrCal.MaximumIterationsPerPoint = value*

Variable (Type) - Description

pwrCal **(object)** - A SourcePowerCalibrator (object)

value **(Long)** – Maximum number of readings. Choose any number between 1 and 100.

Return Type Long Integer

Default 5

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.MaximumIterationsPerPoint = 5 'Write
MaxReads = powerCalibrator.MaximumIterationsPerPoint 'Read
```

C++ Syntax HRESULT get_MaximumIterationsPerPoint(long *pVal);
HRESULT put_MaximumIterationsPerPoint(long newVal);

Interface ISourcePowerCalibrator3

MaximumNumberOfPoints Property

Description Returns the maximum possible number of data points.

VB Syntax `value = cap.MaximumNumberOfPoints`

Variable **(Type) - Description**

`value` **(Long)** - Variable to store the returned maximum value for number of points.

`cap` A [Capabilities](#) **(object)**

Return Type Long

Default Not Applicable

Examples `value = cap.MaximumNumberOfPoints 'Read`

C++ Syntax HRESULT get_MaximumNumberOfPoints(double *
maximumNumberOfPoints);

Interface ICapabilities

MaximumReceiverStepAttenuator Property

Description Returns the maximum amount of receiver attenuation.

VB Syntax `value = cap.MaximumReceiverStepAttenuator (n)`

Variable (Type) - Description

`value` **(Double)** - Variable to store the returned value of maximum receiver attenuation.

`cap` A Capabilities **(object)**

`n` **(Long)** - port number to query for step attenuators

Return Type Double

Default Not Applicable

Examples `value = cap.MaximumReceiverStepAttenuator 'Read`

C++ Syntax HRESULT get_MaximumReceiverStepAttenuator(long portNumber, double * attenuation);

Interface ICapabilities

MaximumSourceALCPower Property

Description Returns a value indicating the maximum amount of source ALC power.

VB Syntax *value* = *cap*.MaximumSourceALCPower (*n*)

Variable **(Type) - Description**

value **(Double)** - Variable to store the returned value for the maximum amount of source ALC power.

cap A [Capabilities](#) **(object)**

n **(Long)** - source number to query for maximum ALC power

Return Type Double

Default Not Applicable

Examples `value = cap.MaximumSourceALCPower 'Read`

C++ Syntax HRESULT get_MaximumSourceALCPower(long sourceNum, double * power);

Interface ICapabilities

MaximumSourceStepAttenuator Property

Description Returns a value for the maximum amount of source attenuation.

VB Syntax *value* = *cap*.MaximumSourceStepAttenuator (*n*)

Variable **(Type) - Description**

value **(Double)** - Variable to store the returned value for the maximum amount of source attenuation.

cap A Capabilities **(object)**

n **(Long)** - port number to query for the maximum amount of source attenuation

Return Type Double

Default Not Applicable

Examples `value = cap.MaximumSourceStepAttenuator 'Read`

C++ Syntax HRESULT get_MaximumSourceStepAttenuator(long portNumber, double * attenuation);

Interface ICapabilities

Read-only

Mean Property

Description Returns the mean value of the measurement . To retrieve all 3 statistics value at the same time, use [meas.GetTraceStatistics](#)

VB Syntax *average* = *meas*.**Mean**

Variable (Type) - Description

average **(single)** - Variable to store mean value

meas A Measurement **(object)**

Return Type Single

Default Not applicable

Examples

```
Dim average as Single
average = meas.Mean 'Read
```

C++ Syntax HRESULT get_Mean(float* mean)

Interface IMeasurement

Medium Property

Description Sets and Returns the media type of the calibration standard.

VB Syntax `calstd.Medium = value`

Variable (Type) - Description

calstd A CalStandard (**object**). Use calKit.[GetCalStandard](#) to get a handle to the standard.

value (**enum** NACalStandardMedium) - Medium of the transmission line of the standard. Choose from:
0 - naCoax - Coaxial Cable
1 - naWaveGuide

Return Type Long Integer

Default Not Applicable

Examples `calstd.Medium = naCoax 'Write`

`stdMedium = calstd.Medium 'Read`

C++ Syntax HRESULT get_Medium(tagNACalStandardMedium *pVal)
HRESULT put_Medium(tagNACalStandardMedium newVal)

Interface ICalStandard

Write/Read

MinimumFrequency Property

Description Sets and Returns the minimum frequency for the calibration standard.

VB Syntax `calstd.MinimumFrequency = value`

Variable (Type) - Description

calstd A CalStandard **(object)**. Use calKit.[GetCalStandard](#) to get a handle to the standard.

value **(double)** -Minimum frequency in Hertz.

Return Type Double

Default Not Applicable

Examples `calstd.MinimumFrequency = 300e3 'Write`

`minFrequency = calstd.MinimumFrequency 'Read`

C++ Syntax HRESULT get_MinimumFrequency(double *pVal)
HRESULT put_MinimumFrequency(double newVal)

Interface ICalStandard

MinimumFrequency Property

Description Returns the minimum frequency of the remote PNA.

VB Syntax `value = cap.MinimumFrequency`

Variable (Type) - Description

`value` (Double) - Variable to store the returned minimum frequency of the PNA.

`cap` A Capabilities (**object**)

Return Type Double

Default Not Applicable

Examples `value = cap.MinimumFrequency 'Read`

C++ Syntax HRESULT get_MinimumFrequency(double *pVal)

Interface ICapabilities

MinimumFrequency (Source Power Cal) Property

Description Minimum usable frequency specified for the power sensor.

VB Syntax *pwrSensor*.MinimumFrequency = *value*

Variable (Type) - Description

pwrSensor **(object)** - A PowerSensor (object)

value **(double)** -Frequency in Hertz.

Return Type Double

Default 0

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.PowerSensors(1).MinimumFrequency = 300e3
'Write

MinFreq = powerCalibrator.PowerSensors(1).MinimumFrequency
'Read
```

C++ Syntax HRESULT put_MinimumFrequency(double newVal);
HRESULT get_MinimumFrequency(double *pVal);

Interface IPowerSensor

MinimumIFFilterSampleCount Property

Description Returns the Minimum allowed value for the [IFFilterSampleCount](#) property for the queried PNA.

Note: An error will occur if this command is used on a PNA without option H08 installed.

VB Syntax *IfConfig*.MinimumIFFilterSampleCount = *value*

Variable **(Type) - Description**

IfConfig [IFConfiguration](#) (object)

value **(long)** The minimum allowed value that can be applied to the [IFFilterSampleCount](#) property.

Return Type Long Integer

Default PNA Model number dependent

Examples

```
variable =
App.ActiveChannel.IFConfiguration.MinimumIFFilterSampleCount
'Read
```

[See an example program](#)

C++ Syntax HRESULT get_MinimumIFFilterSampleCount(long * pMinSampleCount);

Interface IIFConfiguration2

MinimumNumberOfPoints Property

Description Returns the minimum possible number of data points for a data trace.

VB Syntax `value = cap.MinimumNumberOfPoints`

Variable (Type) - Description

value (Long) - Variable to store the returned minimum value for number of points.

cap A [Capabilities](#) (**object**)

Return Type Long

Default Not Applicable

Examples `value = cap.MinimumNumberOfPoints 'Read`

C++ Syntax HRESULT get_MinimumNumberOfPoints(double *
minimumNumberOfPoints);

Interface ICapabilities

MinimumReceiverStepAttenuator Property

Description Returns a value indicating the minimum amount of receiver attenuation.

VB Syntax `value = cap.MinimumReceiverStepAttenuator (n)`

Variable (Type) - Description

`value` **(Double)** - Variable to store the returned minimum value of receiver attenuation.

`cap` A Capabilities **(object)**

`n` **(Long)** - port number to query for minimum value of receiver attenuation

Return Type Double

Default Not Applicable

Examples `value = cap.MinimumReceiverStepAttenuator 'Read`

C++ Syntax `HRESULTget_MinimumReceiverStepAttenuator(long portNumber, double * attenuation);`

Interface ICapabilities

MinimumSourceALCPower Property

Description Returns a value indicating the minimum amount of source ALC power.

VB Syntax `value = cap.MinimumSourceALCPower (n)`

Variable **(Type) - Description**

`value` **(Double)** - Variable to store the returned minimum value of source ALC power.

`cap` A [Capabilities](#) **(object)**

`n` **(Long)** - source number to query for the minimum value of source ALC power

Return Type Double

Default Not Applicable

Examples `value = cap.MinimumSourceALCPower 'Read`

C++ Syntax HRESULT get_MinimumSourceALCPower(long sourceNum, double * power);

Interface ICapabilities

Write/Read

Name (Measurement) Property

Description Sets (or returns) the Name of the measurement. Measurement names must be unique among the set of measurements. Measurement names cannot be an empty string.

Note: This is the same name as trace.Name; when one changes, the other changes.

VB Syntax *meas.Name = value*

Variable (Type) - Description

meas A Measurement (**object**)

value (**string**) - A user defined name of the measurement

Return Type String

Default "CH1_S11_1" - name of the default measurement

Examples `meas.Name = "Filter BPass" 'Write`

`MName = meas.Name 'Read`

C++ Syntax HRESULT get_Name(BSTR *pVal)
HRESULT put_Name(BSTR newVal)

Interface IMeasurement

Write/Read

Name (trace) Property

Description Sets or returns the name of the Trace. Use the trace name to identify the trace and refer to the trace in the collection.

Note: This is the same name as meas.Name; when one changes, the other changes.

VB Syntax *trac.Name = value*

Variable **(Type) - Description**

trac A Trace **(object)**

value **(String)** Trace name

Return Type String

Default "CH1_S11_1" - name of the default measurement

Examples `trace.Name = "myTrace" 'Write`

`traceName = Name.Trace 'Read`

C++ Syntax HRESULT put_Name(BSTR name)
HRESULT get_Name(BSTR *name)

Interface ITrace

Write/Read

Name (CalKit) Property

Description Sets and Returns a name for the selected calibration kit.

VB Syntax *calKit.Name = value*

Variable **(Type) - Description**

calKit A CalKit (**object**).

value (**string**) -Calibration Kit name. Any string name, can include numerics, period, and spaces; any length (although the dialog box display is limited to about 30 characters).

Return Type String

Default Not Applicable

Examples `calKit.Name = "MyCalKit" 'Write`

`KitName = calKit.Name 'Read`

C++ Syntax HRESULT get_Name(BSTR *pVal)
HRESULT put_Name(BSTR newVal)

Interface ICalKit

Read-only

Number (Measurement) Property

Description Returns the Number of the measurement. Measurement numbers are assigned internally.

Note: Measurement numbers are NOT the same as their number in the Measurements collection. Measurement number is used to identify the measurement associated with an event.

This property is used to identify measurements when events occur through the [OnMeasurementEvent](#) callback. For example:

```
OnMeasurementEvent (naEventId_MSG_LIMIT_FAILED, 3)
```

VB Syntax *measNum* = *meas.Number*

Variable **(Type) - Description**

measNum **(long)** - variable to store the measurement number

meas A Measurement **(object)**

Return Type Long Integer

Default "1" - number of the default measurement

Examples `measNum = meas.Number`

C++ Syntax HRESULT get_Number(long *MeasurementNumber)

Interface IMeasurement

NumberOfPoints Property

Description Sets or returns the Number of Points of the channel.
 Sets or returns the Number of Points of the segment.
 See also Measurement2 interface

VB Syntax *object*.**NumberOfPoints** = *value*

Variable (Type) - Description

object Channel **(object)**
or
 CalSet **(object)** - Read-only property

value **(long)** - Number of Points.
 For channel, choose any number from **1** to **16001**.
 For segment, the total number of points in all segments cannot exceed **16001**. A segment can have as few as 1 point.

Return Type Long Integer

Default 201 for channel
 21 for segment

Examples `chan.NumberOfPoints = 201 'sets the number of points for all measurements in the channel. -Write`

`numofpts = chan.NumberOfPoints 'Read`

C++ Syntax HRESULT get_NumberOfPoints(long *pVal)
 HRESULT put_NumberOfPoints(long newVal)

Interface IChannel
 ISegment
 |CalSet3

Read-only

NumberOfPoints Property

Description Returns the number of data points of the measurement. To understand how this property is useful, see [IMeasurement2 Interface](#).

VB Syntax *value* = *meas*.**NumberOfPoints**

Variable (Type) - Description

value **(Long)** - variable to store the returned value

meas A Measurement **(object)**

Return Type Long Integer

Default Not Applicable

Examples `Print meas.NumberOfPoints 'prints the number of data points`

C++ Syntax HRESULT get_NumberOfPoints(long *pVal);

Interface IMeasurement2

Read-only

NumberOfPorts Property

Description Returns the number of hardware source ports on the PNA.

VB Syntax *value* = *app*.NumberOfPorts

Variable (Type) - Description

app An Application (**object**)

value (**long integer**) - variable to contain the returned value

Return Type (long integer)

Default Not Applicable

Examples `iNumPorts = app.NumberOfPorts`

C++ Syntax HRESULT NumberOfPorts(long* NumPorts)

Interface IApplication

NumberOfPorts Property

Description Reads the number of ports (7 or 9) that are on the specified E5091A Testset. Returns 0 if no test set is connected.

VB Syntax *value* = *testsets(1)*.NumberOfPorts

Variable **(Type) - Description**

value (Long) variable to store the returned information (either the number 7 or 9).

testsets(1) An item from [Testsets](#) (**collection**)
Learn how to [identify a testset in the collection](#).

Return Type Long Integer

Default Not Applicable

Examples `value = testset1.NumberOfPorts`

[See Example Program](#)

C++ Syntax HRESULT get_NumberOfPorts(long *numberOfPorts);

Interface IE5091Testsets

Read/Write

OmitIsolation Property

Description Sets and returns whether Isolation portion of the calibration will be performed or not.

VB Syntax *obj.OmitIsolation = bool*

Variable (Type) - Description

obj SMCType (object)

or

VMCType (object)

bool (Boolean)

1 - Isolation is NOT performed

0 - Isolation is performed

Return Type Boolean

Default 1

Examples `value = SMC.OmitIsolation`

C++ Syntax HRESULT put_OmitIsolation (VARIANT_BOOL bState)
HRESULT get_OmitIsolation (VARIANT_BOOL *bState)

Interface SMCType
VMCType

OneReadoutPerTrace Property

Description Either show marker readout of only the active trace or all of the traces simultaneously.

VB Syntax `win.OneReadoutPerTrace = state`

Variable **(Type) - Description**

win A NAWindow (object)

value **(boolean)**

True (1) - Shows the readout of only the active marker for each trace.

False (0) - Shows up to 5 marker readouts per trace, up to 20 total readouts.

Return Type Boolean

Default False (0)

Examples `win.OneReadoutPerTrace = True 'Write`

`State = app.ActiveNAWindow.OneReadoutPerTrace 'Read`

C++ Syntax HRESULT get_OneReadoutPerTrace(VARIANT_BOOL *pVal)
HRESULT put_OneReadoutPerTrace(VARIANT_BOOL newVal)

Interface INAWindow

Options Property

Description Returns a string identifying the analyzer option configuration.

VB Syntax *value* = *app.Options*

Variable **(Type) - Description**

app An [Application](#) (**object**)

value (**string**) - variable to contain the returned string

Return Type String

Default Not Applicable

Examples `availOptions = app.Options`

C++ Syntax HRESULT Options(BSTR* OptionString)

Interface IApplication

OrientECALModule Property

Description Specifies if the PNA should perform orientation of the ECal module during calibration. Orientation is a technique by which the PNA automatically determines which ports of the module are connected to which ports of the PNA. Orientation begins to fail at very low power levels or if there is much attenuation in the path between the PNA and the ECal module.

Note: For 3-port or 4-port measurements, when Orient is OFF, you are not allowed to specify how the ECAL module is connected. Instead, the PNA determines the orientation. Use `cal.OrientECALModule` to query the orientation. The PNA does not verify that you made the connection properly.

VB Syntax `cal.OrientECALModule = value`

Variable **(Type) - Description**

`cal` A Calibrator (**object**)

`value` (**boolean**)

False (0) – DoECAL1Port and DoECAL2Port methods will use the value of the ECALPortMap property to determine the port connections.

True (1) - DoECAL1Port and DoECAL2Port methods will use Orientation technique to determine port connections.

Return Type Boolean

Default True (1)

Examples

```
Dim cal As Calibrator
Dim bOrient As Boolean
Set cal = PNAapp.ActiveChannel.Calibrator
cal.OrientECALModule = False 'Write
bOrient = cal.OrientECALModule 'Read
```

C++ Syntax `HRESULT put_OrientECALModule(VARIANT_BOOL bOrient);`
`HRESULT get_OrientECALModule(VARIANT_BOOL *bOrient);`

Interface ICalibrator3

OutputFixedFrequency Property

Description Sets or returns the mixer output fixed frequency value. This command can only be used with SMC (not VMC) measurements.

VB Syntax *mixer*.OutputFixedFrequency = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

value **(double)** - Output Fixed Frequency in Hertz.

Return Type Double

Default Not Applicable

Examples `Print mixer.OutputFixedFrequency` 'prints the output fixed frequency value of the mixer.'

C++ Syntax HRESULT get_OutputFixedFrequency(double *pVal)
HRESULT put_OutputFixedFrequency(double newVal)

Interface IMixer3

OutputPort Property

Description Switches an input to one of the valid outputs on the specified E5091A. The following are valid input/output combinations. If a combination other than these are sent, an “invalid argument” error will occur.

Input	Valid Outputs
1	A
	T1 - If Port 2 already is connected to T1, then Port 2 will be switched to T2.)
2	T1 - If Port 1 already is connected to T1, then Port 1 will be switched to A.
	T2
3	R1+
	R2+
	R3+ If option 007 (7port), R2 is selected.
4	R1-
	R2-
	R3- If option 007 (7port), R2 is selected.

VB Syntax *testsets(1).OutputPort (chNum,input) = output*

Variable **(Type) - Description**

testsets(1) An item from Testsets (**collection**)
Learn how to identify a testset in the collection.

chNum (**Long**) Channel number of the measurement.

input (**Long**) Testset Input port. Choose from 1|2|3|4.

output (Enum as NAE5091OutputPort) Output port to switch to specified Input. Choose from:

0 or **naE5091PortA** - Port A

1 or **naE5091PortT1** - Port T1

2 or **naE5091PortT2** - Port T2

3 or **naE5091PortR1** - Port R1

4 or **naE5091PortR2** - Port R2

5 or **naE5091PortR3** - Port R3

Return Type Enum

Default Not Applicable

Examples [See Example Program](#)

C++ Syntax HRESULT get_OutputPort(long channelNum, long inputPort, E5091OutputPort *outPort);
HRESULT put_OutputPort(long channelNum, long inputPort, E5091OutputPort outPort);

Interface IE5091Testsets

OutputSideband Property

Description Sets or returns the value of the output sideband, high or low.

VB Syntax `mixer.OutputSideband = value`

Variable (Type) - Description

`mixer` A Mixer **(object)**

`value` **(FCASideBand)** -

Choose from:

0 - LOW

1 - HIGH

Return Type FCASideBand

Default LOW

Examples `Print mixer.OutputSideband 'prints the value of the OutputSideband`

C++ Syntax HRESULT get_OutputSideband(FCASideBand *pVal)
HRESULT put_OutputSideband(FCASideBand newVal)

Interface IMixer

OutputStartFrequency Property

Description Sets or returns the mixer output start frequency.

VB Syntax *mixer*.OutputStartFrequency = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

value **(double)** - Output Start Frequency in Hertz.

Return Type Double

Default Not Applicable

Examples `Print mixer.OutputStartFrequency` 'prints the value of the OutputStartFrequency

C++ Syntax HRESULT get_OutputStartFrequency(double *pVal)
HRESULT put_OutputStartFrequency(double newVal)

Interface IMixer

OutputStopFrequency Property

Description Sets or returns the mixer Output Stop frequency.

VB Syntax *mixer*.OutputStopFrequency = *value*

Variable (Type) - Description

mixer A Mixer **(object)**

value **(double)** - Output stop frequency in Hertz.

Return Type Double

Default Not Applicable

Examples `Print mixer.OutputStopFrequency` 'prints the value of the OutputStopFrequency

C++ Syntax HRESULT get_OutputStopFrequency(double *pVal)
HRESULT put_OutputStopFrequency(double newVal)

Interface IMixer

Read-only

Parameter Property

Description Returns the measurement Parameter. To change the parameter, use `meas.ChangeParameter`

VB Syntax `measPar = meas.Parameter`

Variable **(Type) - Description**

`measPar` **(string)** - Variable to store Parameter string

`meas` A Measurement **(object)**

Return Type String

Default Not applicable

Examples `measPar = meas.Parameter 'Read`

C++ Syntax HRESULT get_Parameter(BSTR *pVal)

Interface IMeasurement

Read-only

Parent Property

Description Returns a handle to the parent object of the collection object being referred to in the statement. The parent property allows the user to traverse from an object back up the object hierarchy.

VB Syntax *object.Parent*

Variable **(Type) - Description**

object Channels collection
Channel object
Measurements collection
NAWindows collection
Traces collection
Segments collection
PowerSensors collection
CalFactorSegments collection
PowerLossSegments collection

Return Type Object

Default Not Applicable

Examples `parentobj = chans.Parent 'returns a handle to the parent object (Application) of the chans collection. -Read`

C++ Syntax HRESULT get_Parent(IApplication* *pApplication); //IChannels, IChannel, IMeasurements and INAWindows
HRESULT get_Parent(IChannel* *pChannel); //ITraces
HRESULT get_Parent(INAWindow* *pWindow); //ISegments
HRESULT get_Parent(IPowerSensor* *pSensor); //ICalFactorSegments
HRESULT get_Parent(ISourcePowerCalibrator* *pCalibrator); //IPowerSensors and IPowerLossSegments

Interface IChannels
IChannel
IMeasurements
INAWindows
ITraces
ISegments
IPowerSensors
ICalFactorSegments
IPowerLossSegments

PassFailLogic Property

Description Sets and reads the logic of the PassFail line on the HANDLER IO connector (pin 33) and AUX IO connector (pin 12). [Learn more about Global Pass/Fail.](#)

Note: This line is connected to both the Handler IO and Aux IO in the PNA. Therefore, this command will affect both of these connectors in the same way.

VB Syntax *object*.PassFailLogic = *value*

Variable **(Type) - Description**

object **(object)** - An Aux I/O or Handler I/O object

value **(enum as NARearPanellIOLogic)** Choose from:

0 - naPositiveLogic - Causes the PassFail line to have positive logic (high = pass, low = fail).

1 - naNegativeLogic - Causes the PassFail line to have negative logic (high = fail, low = pass).

Return Type Long Integer

Default naPositiveLogic

Examples

```
aux.PassFailLogic = naNegativeLogic 'Write
Text1.Text = aux.PassFailLogic 'Read
```

C++ Syntax

```
HRESULT put_PassFailLogic ( tagNARearPanellIOLogic Mode );
HRESULT get_PassFailLogic ( tagNARearPanellIOLogic* Mode );
```

Interface

```
IHWAuxIO
IHWMaterialHandlerIO
```

PassFailMode Property

Description Sets and reads the mode of the PassFail line on the HANDLER IO connector (pin 33) and AUX IO connector (pin 12). [Learn more about Global Pass/Fail.](#)

Note: This line is connected to both the Handler IO and Aux IO in the PNA. Therefore, this command will affect both of these connectors in the same way.

VB Syntax `object.PassFailMode = value`

Variable **(Type) - Description**

object **(object)** - An Aux I/O or Handler I/O object

value **(enum as NAPassFailMode).** Choose from:
0 - naDefaultPassNoWaitMode- the line stays in PASS state. When a device fails, then the line goes to fail IMMEDIATELY.
1 - naDefaultPassWaitMode - the line stays in PASS state. When a device fails, then the line goes to fail after the Sweep End line is asserted.
2 - naDefaultFailWaitMode- the line stays in FAIL state. When a device passes, then the line goes to PASS state after the Sweep End line is asserted.

Return Type Long Integer

Default 0 - naDefaultPassNoWaitMode

Examples

```
HWAuxIO.PassFailMode = naDefaultPassNoWaitMode 'Write
mode = HWAuxIO.PassFailMode 'Read
```

C++ Syntax HRESULT put_PassFailMode (tagNAPassFailMode Mode);
 HRESULT get_PassFailMode (tagNAPassFailMode* Mode);

Interface IHWAuxIO
 IHWMaterialHandlerIO

PassFailPolicy Property

Description	Sets the policy used to determine how global pass/fail is computed. Learn more about Global Pass/Fail.
VB Syntax	<i>object</i> .PassFailPolicy = <i>value</i>
Variable	(Type) - Description
<i>object</i>	(object) - An Aux I/O or Handler I/O object
<i>value</i>	(enum as NAPassFailPolicy) Choose from: 0 - naPolicyAllTests - - Pass/Fail Status returns PASS if all tests on all measurements pass. 1 - naPolicyAllMeas - Pass/Fail Status returns PASS if all measurements have associated tests, and all tests pass. FAIL is returned if even one measurement has no associated limit test. Only those measurements which are not in HOLD mode contribute to the pass/fail result.
Return Type	Long Integer
Default	naPolicyAllTests
Examples	<pre>matHndler.PassFailPolicy = naPolicyAllTests 'Write policy = aux.PassFailPolicy 'Read</pre>
C++ Syntax	HRESULT put_PassFailPolicy (tagNAPassFailPolicy Policy); HRESULT get_PassFailPolicy (tagNARearPanelIOLogic* Policy);
Interface	IHWAuxIO4 IHWMaterialHandlerIO2

PassFailScope Property

Description	Sets and reads the Scope of the PassFail line on the <u>HANDLER IO connector</u> (pin 33) and <u>AUX IO connector</u> (pin 12). Learn more about Global Pass/Fail.
	Note: The PassFail line is connected to both the Handler IO and Aux IO in the PNA. Therefore, this command will affect both of these connectors in the same way.
VB Syntax	<i>object</i> . PassFailScope = <i>value</i>
Variable	(Type) - Description
<i>object</i>	(object) - An Aux I/O or Handler IO object
<i>value</i>	(enum NAPassFailScope) Choose from: 0 - naChannelScope - The PassFail line returns to its default state before sweeps on the next channel start. (A channel measurement may require several sweeps.) 1 - naGlobalScope - The PassFail line returns to its default state before the sweeps for the next triggerable channel start. The default state of the PassFail line before a measurement occurs and after a failure occurs is set by the <u>PassFailMode</u> property.
Return Type	enum NAPassFailScope
Default	1 - naGlobalScope
Examples	<pre>HWAuxIO.PassFailScope = naGlobalScope 'Write scope = HWAuxIO.PassFailScope 'Read</pre>
C++ Syntax	<pre>HRESULT put_PassFailScope (tagNAPassFailScope Scope); HRESULT get_PassFailScope (tagNAPassFailScope* Scope);</pre>
Interface	IHWAuxIO IHWMaterialHandlerIO

PassFailStatus Property

Description Returns the most recent pass/fail status value. Use this command as follows:

1. Set the PNA trigger scope to GLOBAL
2. Set the PNA trigger source to MANUAL or EXTERNAL.
3. Configure and enable Limit Testing
4. Trigger the PNA.
5. Use the *OPC? (with SCPIStringParser object) to determine when the sweep is complete.
6. Use the **PassFailStatus** property to obtain the global pass/fail result.

[Learn more about Global Pass/Fail.](#)

VB Syntax `var = object.PassFailStatus`

Variable **(Type) - Description**

`var` (enum as `NAPassFailStatus`) Variable to store returned status. One of the following will be returned:

0 - naStatusFail - all measurements not in HOLD mode have been swept, and one or more limit tests failed according to the specified Pass/Fail policy.

1 - naStatusPass - all measurements not in HOLD mode have been swept, and all associated limit tests have passed.

2 - naStatusNone - status cannot be determined because measurements are in progress.

`object` **(object)** - An Aux I/O or Handler I/O object

Return Type Long Integer

Default Not Applicable

Examples `status = aux.PassFailStatus 'Read`

C++ Syntax `HRESULT get_PassFailPolicy (tagNAPassFailStatus* status);`

Interface `IHWAuxIO4`
`IHWMaterialHandlerIO2`

Write/Read

PeakExcursion Property

Description Sets and reads the peak excursion value for the specified marker. The Excursion value determines what is considered a "peak".

VB Syntax `mark.PeakExcursion = value`

Variable **(Type) - Description**

mark A Marker (**object**)

value (**single**) - Peak Excursion. Choose any number between **-500** and **500**

Return Type Single

Default 3

Examples `mark.PeakExcursion = 1 'Write`

```
PkExcur = mark.PeakExcursion 'Read
```

C++ Syntax HRESULT get_PeakExcursion(float *pVal)
HRESULT put_PeakExcursion(float newVal)

Interface IMarker

Write/Read

PeakThreshold Property

Description Sets peak threshold for the specified marker. If a peak (using the criteria set with [PeakExcursion](#)) is below this reference value, it will not be considered when searching for peaks.

VB Syntax `mark.PeakThreshold = value`

Variable (Type) - Description

mark A Marker (**object**)

value (**single**) - Peak Threshold. Choose any number between: **-500** and **500**

Return Type Single

Default -100db

Examples `mark.PeakThreshold = 1 'Write`

```
PkThresh = mark.PeakThreshold 'Read
```

C++ Syntax HRESULT get_PeakThreshold(float *pVal)
HRESULT put_PeakThreshold(float newVal)

Interface IMarker

PeakToPeak Property

Description Returns the Peak to Peak value of the measurement. To retrieve all 3 statistics value at the same time, use [meas.GetTraceStatistics](#)

VB Syntax `pp = meas.PeakToPeak`

Variable **(Type) - Description**

`pp` **(single)** - Variable to store peak-to-peak value

`meas` A Measurement **(object)**

Return Type Single

Default Not applicable

Examples `pp = meas.PeakToPeak 'Read`

C++ Syntax HRESULT get_PeakToPeak(float* pp)

Interface IMeasurement

Write/Read

PhaseOffset Property

Description Sets the Phase Offset for the active channel.

VB Syntax `meas.PhaseOffset = value`

Variable **(Type) - Description**

meas A Measurement (**object**)

value **(double)** - PhaseOffset in degrees. Choose any number between: **-360** and **+360**

Return Type Double

Default 0

Examples `meas.PhaseOffset = 25 'Write`

`poffset = meas.PhaseOffset 'Read`

C++ Syntax HRESULT get_PhaseOffset(double *pVal)
HRESULT put_PhaseOffset(double newVal)

Interface IMeasurement

Write/Read

Port1 Property OBSOLETE

Description	This command is replaced by PortDelay property. Sets a Port Extension value for Port 1
VB Syntax	<code>portExt.Port1 = value</code>
Variable	(Type) - Description
<code>portExt</code>	A Port Extension (object)
<code>value</code>	(double) - Port Extension value in seconds. Choose any number between -10 and 10
Return Type	Double
Default	0
Examples	<pre>portExt.Port1 = 10e-6 'Write prt1 = portExt.Port1 'Read</pre>
C++ Syntax	HRESULT get_Port1(double *pVal) HRESULT put_Port1(double newVal)
Interface	IPortExtension

Port2 Property OBSOLETE

Description	<u>This command is replaced by PortDelay property.</u> Sets a Port Extension value for Port 2
VB Syntax	<i>portExt.Port2 = value</i>
Variable	(Type) - Description
<i>portExt</i>	A Port Extension (object)
<i>value</i>	(double) - Port Extension value in seconds. Choose any number between -10 and 10
Return Type	Double
Default	0
Examples	<pre>portExt.Port2 = 10e-6 'Write prt2 = portExt.Port2 'Read</pre>
C++ Syntax	HRESULT get_Port2(double *pVal) HRESULT put_Port2(double newVal)
Interface	IPortExtension

Write/Read

Port3 Property OBSOLETE

Description	This command is replaced by PortDelay property. Sets a Port Extension value for Port 3
VB Syntax	<code>portExt.Port3 = value</code>
Variable	(Type) - Description
<code>portExt</code>	A Port Extension (object)
<code>value</code>	(double) - Port Extension value in seconds. Choose any number between -10 and 10
Return Type	Double
Default	0
Examples	<pre>portExt.Port3 = 10e-6 'Write</pre> <pre>prt3 = portExt.Port3 'Read</pre>
C++ Syntax	HRESULT get_Port3(double *pVal) HRESULT put_Port3(double newVal)
Interface	IPortExtension

Port2PdeembedCktModel Property

Description Select whether or not to load a 2-port De-embedding circuit model for the specified port number. Circuit model is applied when both "USER" is selected and the filename is specified. To set the filename, use [strPort2Pdeembed_S2PFile Property](#)

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.Port2PdeembedCktModel(port) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`port` (**Integer**) Port number to receive circuit model.

`value` (**Enum as NAFixturing2PdeembedCkt**)

0 **naFix2PD_USER** load a 2-port De-embedding circuit model

1 **naFix2PD_NONE** no model

Return Type Long Integer

Default naFix2PD_NONE

Examples `fixture.Port2PdeembedCktModel(2) = naFix2PD_USER 'Write`

`value = fixture.Port2PdeembedCktModel(1) 'Read`

C++ Syntax HRESULT get_Port2PdeembedCktModel(short port tagNAFixturing2PdeembedCkt *pVal)
 HRESULT put_Port2PdeembedCktModel(short port tagNAFixturing2PdeembedCkt newVal)

Interface IFixturing

Port2PdeembedState Property

Description Turns de-embedding ON or OFF for all ports on the channel.

VB Syntax `fixture.Port2PdeembedState = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`value` (**Boolean**)

False - Turns De-embedding OFF

True - Turns De-embedding ON

Return Type Boolean

Default False (OFF)

Examples `fixture.Port2PdeembedState = 0 'Write`

`value = fixture.Port2PdeembedState 'Read`

C++ Syntax HRESULT get_Port2PdeembedState(VARIANT_BOOL *pVal)
HRESULT put_Port2PdeembedState(VARIANT_BOOL newVal)

Interface IFixturing

PortArbzImag Property

Description Sets and returns the Imaginary portion of the impedance value for the specified single-ended port. Use [PortArbzReal](#) to set the real value. Or use [PortArbzZ0](#) to set both values together.

VB Syntax `fixture.PortArbzImag(portNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`portNum` (**Integer**) Single-ended port number to receive impedance value.

`value` (**Double**) Real Impedance value. Choose a value between -1E18 and 1E18

Return Type Double

Default 0

Examples `fixture.PortArbzImag(2) = 75 'Write`

`value = fixture.PortArbzImag(1) 'Read`

C++ Syntax HRESULT get_PortArbzImag(short portNum, double *pVal)
 HRESULT put_PortArbzImag(short portNum, double newVal)

Interface IFixturing3

PortArbzReal Property

Description Sets and returns the Real portion of the impedance value for the specified single-ended port. Use [PortArbzImag](#) to set the imaginary value. Or use [PortArbzZ0](#) to set both values together.

VB Syntax `fixture.PortArbzReal(portNum) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (object)

`portNum` (**Integer**) Single-ended port number to receive impedance value.

`value` (**Double**) Real Impedance value. Choose a value between 0 to 1E7

Return Type Double

Default 50

Examples `fixture.PortArbzReal(2) = 75 'Write`

`value = fixture.PortArbzReal(1) 'Read`

C++ Syntax HRESULT get_PortArbzReal(short portNum, double *pVal)
HRESULT put_PortArbzReal(short portNum, double newVal)

Interface IFixturing3

PortArbzState Property

Description Turns Port Impedance ON or OFF for all ports on the channel.

VB Syntax `fixture.PortArbzState = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`value` (**Boolean**)

False - Turns Port Impedance OFF

True - Turns Port Impedance ON

Return Type Boolean

Default False (OFF)

Examples `fixture.PortArbzState = 0 'Write`

`value = fixture.PortArbzState 'Read`

C++ Syntax HRESULT get_PortArbzState(VARIANT_BOOL *pVal)
HRESULT put_PortArbzState(VARIANT_BOOL newVal)

Interface IFixturing

PortArbzZ0 Property

Description Sets and returns the Real portion of the impedance value for the specified single-ended port. The imaginary portion is automatically set to 0.0.

To set both values separately, use [PortArbzReal](#) and [PortArbzImag](#).

VB Syntax `fixture.PortArbzZ0(portNum) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`portNum` (**Integer**) Single-ended port number to receive impedance value.

`value` (**Double**) Impedance value. Choose a value between 0 to 1E7

Return Type Double

Default 50

Examples `fixture.PortArbzZ0(2) = 75 'Write`

`value = fixture.PortArbzZ0(1) 'Read`

C++ Syntax HRESULT get_PortArbzZ0(short portNum, double *pVal)
HRESULT put_PortArbzZ0(short portNum, double newVal)

Interface IFixturing3

Read/Write

PortCLogic Property

Description Sets and reads the logic mode of Port C on the AUX IO connector and the Handler IO connector.

Note: Port C lines are connected to both the Handler IO and Aux IO in the PNA. Therefore, this command will affect both of these connectors in the same way.

VB Syntax *AuxIO.PortCLogic = value*

Variable **(Type) - Description**

AuxIO **(object)** - A Hardware Aux I/O object

value **(Enum as NaRearPanelIOLogic)** - Choose from:

0 - naPositiveLogic - The associated data line goes **HIGH** when writing a 1 to a PortC bit.

1 - naNegativeLogic - The associated data line goes **LOW** when writing a 1 to a PortC bit.

When Port C is in Output/Write mode, a change in logic causes the output lines to change state immediately. For example, Low levels change to High levels.

When Port C is in Input/Read mode, a change in logic will not cause the lines to change, but data read from Port C will reflect the change in logic.

Return Type Enum

Default 1 - naNegativeLogic

Examples

```
auxIO.PortCLogic = value 'Write
value = auxIo.PortCLogic 'Read
```

C++ Syntax HRESULT put_PortCLogic (tagNARearPanelIOLogic Mode);
 HRESULT get_PortCLogic (tagNARearPanelIOLogic* Mode);

Interface IHWAuxIO

Read/Write

PortCMode Property

Description Sets and reads whether Port C is setup for writing or reading data on the AUX IO connector and the Handler IO connector.

Note: Port C lines are connected to both the Handler IO and Aux IO in the PNA. Therefore, this command will affect both of these connectors in the same way.

VB Syntax *AuxIO.PortCMode = value*

Variable **(Type) - Description**

AuxIO **(object)** - A Hardware Aux I/O object

value **(enum as NaPortMode)** - Choose from:

0 - naInput - set the port for reading

1 - naOutput - set the port for writing

Return Type Enum as NaPortMode

Default 1 - naInput

Examples `auxIo.get_PortCMode = naInput 'Write`

`value = auxIo.get_PortCMode 'Read`

C++ Syntax `HRESULT get_PortCMode(tagNAPortMode* pMode);`
`HRESULT put_PortCMode(tagNAPortMode pMode);`

Interface IHWAuxIO

PortDelay Property

Description Sets and returns the Port Extensions Delay value for the specified port number.

Note: This command affects ALL measurements on the channel.

This command replaces Port 1 Port 2 Port 3 Properties.

VB Syntax *fixture.PortDelay(port) = value*

Variable (Type) - Description

fixture A Fixturing (**object**)

port (**Integer**) Port number to receive delay value.

value (**Double**) Delay value in seconds. Choose a value between -1E18 and 1E18.

Return Type Double

Default 0

Examples `fixture.PortDelay(2) = .002 'Write`

`value = fixture.PortDelay(1) 'Read`

C++ Syntax HRESULT get_PortDelay(short port double *pVal)
HRESULT put_PortDelay(short port double newVal)

Interface IFixturing

PortExtState Property

Description Turns Port Extension ON or OFF for all ports on the channel.

VB Syntax `fixture.PortExtState = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`value` (**Boolean**)

False - Turns Port Extensions OFF

True - Turns Port Extensions ON

Return Type Boolean

Default False

Examples `fixture.PortExtState = 0 'Write`

`value = fixture.PortExtState 'Read`

C++ Syntax HRESULT get_PortExtState(VARIANT_BOOL *pVal)
HRESULT put_PortExtState(VARIANT_BOOL newVal)

Interface IFixturing

PortExtUse1 Property

Description Sets and returns the Use1 ON/OFF state for the use of the [PortLoss1](#) and [PortFreq1](#) values for the specified port number.

[Learn about Loss compensation values.](#)

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortExtUse1(port) = value`

Variable (Type) - Description

fixture A [Fixturing](#) (**object**)

port (**Integer**) Port number to receive Use1 ON / OFF state.

value (**Boolean**)

False - Turns Use1 OFF

True - Turns Use1 ON

Return Type Boolean

Default False (OFF)

Examples `fixture.PortExtUse1(2) = 0 'Write`

`value = fixture.PortExtUse1(1) 'Read`

C++ Syntax HRESULT get_PortExtUse1(short port VARIANT_BOOL *pVal)
 HRESULT put_PortExtUse1(short port VARIANT_BOOL newVal)

Interface IFixturing

PortExtUse2 Property

Description Sets and returns the Use2 ON/OFF state for the use of the PortLoss2 and PortFreq2 values for the specified port number.

[Learn about Loss compensation values.](#)

Note: This command affects ALL measurements on the channel.

VB Syntax *fixture.PortExtUse2(port) = value*

Variable (Type) - Description

fixture A Fixturing (**object**)

port (**Integer**) Port number to receive Use2 ON / OFF state.

value (**Boolean**)

False - Turns Use1 OFF

True - Turns Use1 ON

Return Type Boolean

Default False (OFF)

Examples `fixture.PortExtUse2(2) = 0 'Write`

`value = fixture.PortExtUse2(1) 'Read`

C++ Syntax HRESULT get_PortExtUse2(short port VARIANT_BOOL *pVal)
 HRESULT put_PortExtUse2(short port VARIANT_BOOL newVal)

Interface IFixturing

PortFreq1 Property

Description Sets and returns Frequency1 value for the specified port number.

[Learn about Loss compensation values.](#)

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortFreq1(port) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`port` (**Integer**) Port number to receive extrapolated loss.

`value` (Double) Frequency1 value. Choose a frequency within the frequency span of the PNA.

Return Type Double

Default 1 GHz

Examples `fixture.PortFreq1(2) = naFix2PD_USER 'Write`

`value = fixture.PortFreq1(1) 'Read`

C++ Syntax HRESULT get_PortFreq1(short port double *pVal)
HRESULT put_PortFreq1(short port double newVal)

Interface IFixturing

PortFreq2 Property

Description Sets and returns Frequency2 value for the specified port number.

[Learn about Loss compensation values.](#)

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortFreq2(port) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`port` (**Integer**) Port number to receive extrapolated loss.

`value` (Double) Frequency2 value. Choose a frequency within the frequency span of the PNA.

Return Type Double

Default 1 GHz

Examples `fixture.PortFreq2(2) = 10E9 'Write`

`value = fixture.PortFreq2(1) 'Read`

C++ Syntax HRESULT get_PortFreq2(short port double *pVal)
HRESULT put_PortFreq2(short port double newVal)

Interface IFixturing

PortLabel Property

Description Sets and returns the label on the calibration kit Port for the calibration wizard.

VB Syntax *calKit*.PortLabel (*portNum*) = *value*

Variable (Type) - Description

calKit A CalKit (**object**)

portNum (**long integer**) - number of the port to be labeled. Choose either **1** or **2**

value (**string**) - Label that is visible in the calibration wizard.

Return Type String

Default Depends on the Cal Kit.

Examples `calKit.PortLabel = "MyCalKit" 'Write`

`kitLabel = calKit.PortLabel 'Read`

C++ Syntax HRESULT get_PortLabel(long port, BSTR *pVal)
HRESULT put_PortLabel(long port, BSTR newVal)

Interface ICalKit

PortLogic Property

Description	Sets and returns the logic mode of data ports A-H on the HandlerIO connector. Port C of the Handler IO is connected internally to the Port C of the Aux IO connector. Therefore, it will have the same logic mode.
VB Syntax	<i>handler</i> .PortLogic = <i>value</i>
Variable	(Type) - Description
<i>handler</i>	(object) - A HandlerI/O object
<i>value</i>	(enum as NaRearPanellIOLogic) - Choose from: 0 - naPositiveLogic - When a value of one is written, the associated line goes High 1 - naNegativeLogic - When a value of one is written, the associated line goes Low For ports that are in output (write) mode, a change in logic causes the output lines to change state immediately. For example, Low levels change immediately to High levels. For ports that are in input (read) mode (C,D,E only), a change in logic will be reflected when data is read from that port. For example, if a line read 0, the next read after a logic change will read 1.
Return Type	Long Integer
Default	1 - naNegativeLogic
Examples	<pre>handler.PortLogic = value 'Write value = handler.PortLogic 'Read</pre>
C++ Syntax	<pre>HRESULT put_PortLogic(tagNARearPanellIOLogic Mode); HRESULT get_PortLogic(tagNARearPanellIOLogic* Mode);</pre>
Interface	IHWMaterialHandlerIO

PortLoss1 Property

Description Sets and returns the Loss1 value for the specified port number.

[Learn about Loss compensation values.](#)

Note: This command affects ALL measurements on the channel.

VB Syntax *fixture.PortLoss1(port) = value*

Variable (Type) - Description

fixture A [Fixturing](#) (**object**)

port (**Integer**) Port number to receive Loss value

value (**Double**) Loss1 value in dB. Choose a value between -90 and 90.

Return Type Double

Default 0

Examples `fixture.PortLoss1(2) = .002 'Write`

`value = fixture.PortLoss1(1) 'Read`

C++ Syntax HRESULT get_PortLoss1(short port double *pVal)
HRESULT put_PortLoss1(short port double newVal)

Interface IFixturing

PortLoss2 Property

Description Sets and returns the Loss2 value for the specified port number.

[Learn about Loss compensation values.](#)

Note: This command affects ALL measurements on the channel.

VB Syntax *fixture.PortLoss2(port) = value*

Variable (Type) - Description

fixture A [Fixturing](#) (**object**)

port (**Integer**) Port number to receive Loss value

value (**Double**) Loss2 value in dB. Choose a value between -90 and 90.

Return Type Double

Default 0

Examples `fixture.PortLoss2(2) = .002 'Write`

`value = fixture.PortLoss2(1) 'Read`

C++ Syntax HRESULT get_PortLoss2(short port double *pVal)
HRESULT put_PortLoss2(short port double newVal)

Interface IFixturing

PortLossDC Property

Description Sets and returns the Loss value at DC for the specified port number.

[Learn about Loss compensation values.](#)

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortLossDC(port) = value`

Variable (Type) - Description

`fixture` A [Fixturing](#) (**object**)

`port` (**Integer**) Port number to receive Loss value at DC.

`value` (**Double**) Loss value in ohms. Choose a value between -90 and 90

Return Type Double

Default 0

Examples `fixture.PortLossDC(2) = .002 'Write`

`value = fixture.PortLossDC(1) 'Read`

C++ Syntax HRESULT get_PortLossDC(short port double *pVal)
HRESULT put_PortLossDC(short port double newVal)

Interface IFixturing

PortMatching_C Property

Description Sets and returns the Capacitance value for the specified port number.

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortMatching_C(port) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) **(object)**

`port` **(Integer)** Port number to receive capacitance value

`value` **(Double)** Capacitance value in farads. Choose a value between -1E18 to 1E18.

Return Type Double

Default 0

Examples `fixture.PortMatching_C(2) = .00002 'Write`

`value = fixture.PortMatching_C(1) 'Read`

C++ Syntax HRESULT get_PortMatching_C(short port double *pVal)
HRESULT put_PortMatching_C(short port double newVal)

Interface IFixturing

PortMatching_G Property

Description Sets and returns the Conductance value for the specified port number.

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortMatching_G(port) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`port` (**Integer**) Port number to receive conductance value.

`value` (**Double**) Conductance value in siemens. Choose a value between -1E18 and 1E18.

Return Type Double

Default 0

Examples `fixture.PortMatching_G = .002 'Write`

`value = fixture.PortMatching_G 'Read`

C++ Syntax HRESULT get_PortMatching_G(short port double *pVal)
HRESULT put_PortMatching_G(short port double newVal)

Interface IFixturing

PortMatching_L Property

Description Sets and returns the Inductance value for the specified port number.

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortMatching_L(port) = value`

Variable **(Type) - Description**

`fixture` A Fixturing **(object)**

`port` **(Integer)** Port number to receive inductance value

`value` **(Double)** Inductance value in henries. Choose a value between -1E18 and 1E18.

Return Type Double

Default 0

Examples `fixture.PortMatching_L = .002 'Write`

`value = fixture.PortMatching_L 'Read`

C++ Syntax HRESULT get_PortMatching_L(short port double *pVal)
HRESULT put_PortMatching_L(short port double newVal)

Interface IFixturing

PortMatching_R Property

Description Sets and returns the Resistance value for the specified port number.

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortMatching_R(port) = value`

Variable **(Type) - Description**

`fixture` A [Fixturing](#) (**object**)

`port` (**Integer**) Port number to receive resistance value.

`value` (**Double**) Resistance value in ohms. Choose a value between -1E18 and 1E18.

Return Type Double

Default 0

Examples `fixture.PortMatching_R = .1 'Write`

`value = fixture.PortMatching_R 'Read`

C++ Syntax HRESULT get_PortMatching_R(short port double *pVal)
HRESULT put_PortMatching_R(short port double newVal)

Interface IFixturing

PortMatchingCktModel Property

Description Sets and returns the Port Matching circuit model for the specified port number.

Note: This command affects ALL measurements on the channel.

VB Syntax `fixture.PortMatchingCktModel(port) = value`

Variable (Type) - Description

`fixture` A Fixturing (**object**)

`port` (**Integer**) Port number to receive circuit model.

`value` (**Enum as NAFixturingPortMatchCkt**) Circuit model. Choose from

0 **naFixPMC_SLPC** Series L - Parallel C

1 **naFixPMC_PCSL** Parallel C - Series L

2 **naFixPMC_PLSC** Parallel L - Series C

3 **naFixPMC_SCPL** Series C - Parallel L

4 **naFixPMC_PLPC** Parallel L - Parallel C

5 **naFixPMC_USER** Load S2P file - also set filename to load with strPortMatch_S2PFile Property

6 **naFixPMC_NONE** No circuit model

Return Type Long Integer

Default **naFixPMC_NONE**

Examples `fixture.PortMatchingCktModel(2) = naFixPMC_PLSC 'Write`

`value = fixture.PortMatchingCktModel(1) 'Read`

C++ Syntax HRESULT get_PortMatchingCktModel(short port tagNAFixturingPortMatchCkt *pVal)
 HRESULT put_PortMatchingCktModel(short port tagNAFixturingPortMatchCkt newVal)

Interface IFixturing

PortMatchingState Property

Description Sets and returns the Port Matching State on the channel.

VB Syntax *fixture*.PortMatchingState = *value*

Variable (Type) - Description

fixture A [Fixturing](#) (**object**)

value **(boolean)**
True (1) - Turns Port Matching ON
False (0) - Turns Port Matching OFF

Return Type Boolean

Default False

Examples `fixture.PortMatchingState = True 'Write`

`value = fixture.PortMatchingState 'Read`

C++ Syntax HRESULT get_PortMatchingState(VARIANT_BOOL *pVal)
HRESULT put_PortMatchingState(VARIANT_BOOL newVal)

Interface IFixturing

PortMode Property

Description	Sets and returns whether Port C or Port D is used for writing or reading data on the Handler IO connector. The Handler IO Port C is connected internally to the Port C of the Aux IO connector. Therefore, the Aux IO connector will have the same input/output mode.
VB Syntax	<i>handler</i> .PortMode (<i>port</i>) = <i>value</i>
Variable	(Type) - Description
<i>handler</i>	(object) - A Handler I/O object
<i>port</i>	(enum as NAmatHandlerPort) Port to be changed. Choose from: 2 - naPortC 3 - naPortD
<i>value</i>	(enum as NaPortMode) - Choose from: 0 - naInput - set the port for reading 1 - naOutput - set the port for writing
Return Type	Long Integer
Default	1 - naInput
Examples	<pre>handler.PortMode(naPortC) = naInput 'Write value = handler.PortMode(naPortD) 'Read</pre>
C++ Syntax	HRESULT put_PortMode (tagNAmatHandlerPort Port, tagNAPortMode Mode); HRESULT get_PortMode (tagNAmatHandlerPort Port, tagNAPortMode* Mode);
Interface	IHWMaterialHandlerIO

PowerSlope Property

Description Sets or returns the Power Slope value. Power Slope function increases or decreases the output power over frequency. Units are db/GHz. For example: PowerSlope = 2 will increase the power 2db/1GHZ.

VB Syntax *object*.PowerSlope = *value*

Variable (Type) - Description

object Channel (**object**)

or

CalSet (**object**) - Read-only property

value (**double**) - Power Slope. Choose any number between -2 and 2.
No slope = 0

Return Type Double

Default 0

Examples `chan.PowerSlope = 2 'Write`

`pwrslp = chan.PowerSlope 'Read`

C++ Syntax HRESULT get_PowerSlope(double *pVal)
HRESULT put_PowerSlope(double newVal)

Interface IChannel
|CalSet3

PowerAcquisitionDevice Property

Description	<p>Returns the power sensor channel (A or B) that is currently selected for use at a specific frequency.</p> <p>If <u>UsePowerSensorFrequencyLimits</u> is set to False, this property will return the sensor channel last used for a source power calibration. This setting corresponds to the Use this sensor only checkbox in the <u>Power Sensor Settings</u> dialog.</p> <p>When performing an SMC calibration, use <u>SetPowerAcquisitionDevice Method</u> to set the power sensor channel.</p>
VB Syntax	<i>sensor</i> = <i>pwrCal</i> .PowerAcquisitionDevice(<i>dFreq</i>)
Variable	(Type) - Description
<i>sensor</i>	(enum NAPowerAcquisitionDevice) The currently selected sensor channel for the specified frequency. Choose from: 0 – naPowerSensor_A 1 – naPowerSensor_B
<i>pwrCal</i>	A SourcePowerCalibrator (object)
<i>dFreq</i>	(double) Frequency (Hz) for the power reading of interest.
Return Type	enum NAPowerAcquisitionDevice
Default	Not Applicable
Examples	<code>selectedSensor = pwrCal.PowerAcquisitionDevice(1.E9) 'Write</code>
C++ Syntax	HRESULT get_PowerAcquisitionDevice(double dFreq, tagNAPowerAcquisitionDevice* enumAcqDevice);
Interface	ISourcePowerCalibrator2

Read-only

PowerMeterChannel Property

Description Identifies which channel of the power meter the power sensor is connected to.

VB Syntax `chan = powerSensor.PowerMeterChannel`

Variable **(Type) - Description**

chan **(enum NAPowerAcquisitionDevice)** – Power meter channel identifier for sensor.
Choose from:

0 – naPowerSensor_A

1 – naPowerSensor_B

pwrSensor **(object)** - A PowerSensor (object)

Return Type NAPowerAcquisitionDevice

Default Not Applicable

Examples

```
Set pwrCal = pna.SourcePowerCalibrator
meterChannel = pwrCal.PowerSensors(1).PowerMeterChannel
```

C++ Syntax HRESULT PowerMeterChannel(tagNAPowerAcquisitionDevice *pSensor);

Interface IPowerSensor

PowerMeterGPIBAddress Property

Description Specifies the GPIB address of the power meter that will be referenced by the SourcePowerCalibrator object.

When performing a source power cal, the PNA will search VISA interfaces that are configured in the Agilent IO Libraries on the PNA.

VB Syntax *powerCalibrator*.**PowerMeterGPIBAddress** = *value*

Variable (Type) - Description

powerCalibrator **(object)** - A SourcePowerCalibrator (object)

value **(long integer)** – Power meter GPIB address. Choose any number between 0 and 30.

Return Type Long integer

Default 13

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.PowerMeterGPIBAddress = 13 'Write

pwrMtrAddress = powerCalibrator.PowerMeterGPIBAddress 'Read
```

C++ Syntax HRESULT put_PowerMeterGPIBAddress(long newVal);
 HRESULT get_PowerMeterGPIBAddress(long *pVal);

Interface ISourcePowerCalibrator

R1inputPath Property

Description PNA models with option 081 have a switch in the test set that allows access to the port 1 reference receiver through the front panel Reference 1 connectors. This command throws that switch between the internal path to the receiver, or through the external connectors. You could use this feature to make converter measurements relative to a reference ("golden") mixer.

See other [Frequency Offset](#) properties.

VB Syntax `chan.R1InputPath = value`

Variable **(Type) - Description**

chan A Channel **(object)**

value **(Enum as naInputPath)** - Choose from: naPathInternal -
(0) - internal path to the reference receiver naPathExternal
(1) - path through external connectors

Return Type Enum

Default naPathInternal - (0)

Examples `chan.R1InputPath = naPathInternal 'Write`

`Inpath = chan.R1InputPath 'Read`

C++ Syntax HRESULT get_R1InputPath (tag NAInputPath *pPath);
 HRESULT put_R1InputPath (tag NAInputPath newPath);

Interface IChannel2

Write / Read

ReadingsPerPoint Property

Description Specifies the maximum number of power readings that are taken at each stimulus point to allow for power meter settling. Each reading is averaged with the previous readings at that stimulus point. When this average meets the ReadingsTolerance value or this number of readings has been made, the average is returned as the valid reading.

VB Syntax *pwrCal.ReadingsPerPoint = value*

Variable **(Type) - Description**

pwrCal **(object)** - A SourcePowerCalibrator (object)

value **(long integer)** – Number of power readings. Choose any number between 3 and 100.

Return Type Long Integer

Default 3

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.ReadingsPerPoint = 3 'Write
numReadings = powerCalibrator.ReadingsPerPoint 'Read
```

C++ Syntax HRESULT put_ReadingsPerPoint(long newVal);
HRESULT get_ReadingsPerPoint(long *pVal);

Interface ISourcePowerCalibrator

Write / Read

ReadingsTolerance Property

Description Each power reading is averaged with the previous readings at each stimulus point. When the average meets this tolerance value or the maximum ReadingsPerPoint has been made, the average is returned as the valid reading.

VB Syntax *pwrCal.ReadingsTolerance = value*

Variable (Type) - Description

pwrCal **(object)** - A SourcePowerCalibrator (object)

value **(Double)** – Power meter settling tolerance value in dB. Choose any number between 0 and 5.

Return Type Double

Default .05 dB

Examples

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.ReadingsTolerance = .1 'Write
ReadTol = powerCalibrator.ReadingsTolerance 'Read
```

C++ Syntax HRESULT get_ReadingsTolerance(double *pVal);
 HRESULT put_ReadingsTolerance(double newVal);

Interface ISourcePowerCalibrator3

ReadyForTriggerState Property

Description Determines the control of Material Handler connector Pin 21.

VB Syntax *handler*.ReadyForTriggerState = *value*

Variable (Type) - Description

handler **(object)** - A Handler I/O object

value **(boolean)**

0 (False) - Pin 21 is controlled by Output Port B7

1(True) - Pin 21 is controlled by the Ready for Trigger signal

Return Type Boolean

Default

Examples `handler.ReadyForTriggerState = False 'Write
bState = handler.ReadyForTriggerState 'Read`

C++ Syntax HRESULT put_ReadyForTriggerState (BOOL *pVal);
HRESULT get_ReadyForTriggerState (BOOL newVal);

Interface IHWMaterialHandlerIO2

ReceiverAttenuator Property

Description	Sets or returns the value of the specified receiver attenuator control.
VB Syntax	<i>object</i> .ReceiverAttenuator(<i>rec</i>) = <i>value</i>
Variable	(Type) - Description
<i>object</i>	Channel (object) or CalSet (object) - Read-only propertyA Channel (object)
<i>rec</i>	(long integer) - Receiver with attenuator control to be changed. Choose from: 1 - Receiver A 2 - Receiver B
<i>value</i>	(double) - Attenuator value in dB. Choose any Long Integer between 0 and 35 in 5dB steps: If an invalid value is entered, the analyzer will select the next lower valid value. For example, if 19.9 is entered the analyzer will select 15 dB attenuation.
Return Type	Double
Default	0 db
Examples	<pre>chan.ReceiverAttenuator(1) = 5 'Write</pre> <pre>attn = chan.ReceiverAttenuator(2) 'Read</pre>
C++ Syntax	HRESULT get_ReceiverAttenuator(long lport, double *pVal) HRESULT put_ReceiverAttenuator(long lport, double newVal)
Interface	IChannel CalSet3

ReceiverCount Property

Description Returns the number of receivers in the remote PNA.

VB Syntax `value = cap.ReceiverCount`

Variable **(Type) - Description**

value (Long) - Variable to store the returned number of receivers.

cap A [Capabilities](#) (**object**)

Return Type Long

Default Not Applicable

Examples `value = cap.ReceiverCount 'Read`

C++ Syntax HRESULT get_ReceiverCount(long * receiverCount);

Interface ICapabilities

ReceiverStepAttenuatorStepSize Property

Description Returns a value indicating the step size of the attenuator.

VB Syntax `value = cap.ReceiverStepAttenuatorStepSize (n)`

Variable **(Type) - Description**

`value` **(Double)** - Variable to store the returned value of the attenuator step size.

`cap` A [Capabilities](#) **(object)**

`n` **(Long)** - port number to query for the value of the attenuator step size.

Return Type Double

Default Not Applicable

Examples `value = cap.ReceiverStepAttenuatorStepSize 'Read`

C++ Syntax HRESULT get_ReceiverStepAttenuatorStepSize(long portNumber, double * stepSize);

Interface ICapabilities

Read-only

ReceivePort Property

Description Returns the receiver (response) port number of measurement. To understand how this property is useful, see [IMeasurement2 Interface](#).

Note: Returning a receiver port is only supported for S-Parameter measurements. If the measurement is not an S-Parameter, then `E_NA_BAD_PARAMETER` is returned.

VB Syntax `value = meas.ReceivePort`

Variable **(Type) - Description**

`value` **(Long)** - Variable to store the returned value

`meas` A [Measurement](#) **(object)**

Return Type Long Integer

Default Not Applicable

Examples `rp = meas.ReceivePort`

C++ Syntax `HRESULT ReceivePort(Long* rcvPort);`

Interface `IMeasurement2`

ReduceIFBW Property

Description Sets or returns the state of the Reduced IF Bandwidth at Low Frequencies setting.

VB Syntax `chan.ReduceIFBW = state`

Variable (Type) - Description

`chan` A Channel (**object**)

`state` (**boolean**)
0 - Turns Reduce IFBW **OFF**
1 - Turns Reduce IFBW **ON**

Return Type Boolean

Default 1

Examples `chan.ReduceIFBW = 1 'Write`

`reduce = chan.ReduceIFBW 'Read`

C++ Syntax HRESULT get_ReduceIFBW(BOOL *pVal)
HRESULT put_ReduceIFBW(BOOL newVal)

Interface IChannel

Read-only

ReferenceCalFactor Property

- Description** Reference cal factor (%) associated with this power sensor. This property and the CalFactorSegments collection are used to perform source power calibration **only** if the power sensor does not contain cal factors in EPROM (for example, HP/Agilent 848x sensors).
- VB Syntax** *powerSensor.ReferenceCalFactor = value*
- Variable (Type) - Description**
- pwrSensor* **(object)** - A PowerSensor (object)
- value* **(double)** – Cal factor in units of percent. This can be any value between 1 and 150.
- Return Type** Double
- Default** 100
- Examples**
- ```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.PowerSensors(1).ReferenceCalFactor = 99 'Write
RefFact = powerCalibrator.PowerSensors(1).ReferenceCalFactor
'Read
```
- C++ Syntax** HRESULT put\_ReferenceCalFactor(double newVal);  
HRESULT get\_ReferenceCalFactor(double \*pVal);
- Interface** IPowerSensor

## ReferenceMarkerState Property

---

**Description** Turn ON or OFF the reference marker.

**VB Syntax** `meas.ReferenceMarkerState = state`

**Variable** (Type) - Description

`app` A Measurement (**object**)

`state` (boolean) -  
ON (1) turns the reference marker ON  
OFF (0) turns the reference marker OFF

**Return Type** Boolean

**Default** 0 - OFF

**Examples** `meas.ReferenceMarkerState = True`

`reference = meas.ReferenceMarkerState`

**C++ Syntax** HRESULT get\_ReferenceMarkerState(VARIANT\_BOOL bState)  
HRESULT put\_ReferenceMarkerState(VARIANT\_BOOL\* bState)

**Interface** IMeasurement



Write/Read

## ReferenceValue Property

---

**Description** Sets or returns the value of the Y-axis Reference Level of the active trace.

**VB Syntax** `trce.ReferenceValue = value`

**Variable** (Type) - Description

*trce* A Trace (**object**)

*value* (**double**) - Reference Value. Units and range depend on the current data format.

**Return Type** Double

**Default** Not applicable

**Examples** `meas.ReferenceValue = 0 'Write`

`rlev = meas.ReferenceValue 'Read`

**C++ Syntax** HRESULT get\_ReferenceValue(double \*pVal)  
HRESULT put\_ReferenceValue(double newVal)

**Interface** ITrace

Write/Read

## ReferencePosition Property

---

**Description** Sets or returns the Reference Position of the active trace.

**VB Syntax** `trce.ReferencePosition = value`

**Variable (Type) - Description**

*trce* A Trace (**object**)

*value* (**double**) - Reference position on the screen measured in horizontal graticules from the bottom of the screen. Choose from any number between: **0** and **10**.

**Return Type** Double

**Default** 0

**Examples** `meas.ReferencePosition = 5 'Middle of the screen -Write`

`rpos = meas.ReferencePosition -Read`

**C++ Syntax** HRESULT get\_ReferencePosition(double \*pVal)  
HRESULT put\_ReferencePosition(double newVal)

**Interface** ITrace

## SB\_BalPortNegative Property

---

**Description** With a Single-ended - Balanced topology, returns the PNA port number that is connected to the Negative side of the DUT's Balanced Port.

Use [SetSBPorts Method](#) to set the port mapping for a Single-Ended - Balanced topology.

**VB Syntax** `var = balTopology.SB_BalPortNegative`

**Variable (Type) - Description**

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `variable = balTop.SB_BalPortNegative 'Read`

**C++ Syntax** HRESULT get\_SB\_BalPortNegative(long \*bVal)

**Interface** IBalancedTopology

## SB\_BalPortPositive Property

---

**Description** With a Single-ended - Balanced topology, returns the PNA port number that is connected to the Positive side of the DUT's Balanced Port.

Use [SetSBPorts Method](#) to set the port mapping for a Single-Ended - Balanced topology.

**VB Syntax** `var = balTopology.SB_BalPortPositive`

**Variable (Type) - Description**

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `variable = balTop.SB_BalPortPositive 'Read`

**C++ Syntax** HRESULT get\_SB\_BalPortPositive(long \*bVal)

**Interface** IBalancedTopology

**SB\_SEPort Property**

---

**Description** With a Single-ended - Balanced topology, returns the PNA port number that is connected to the DUT's Single-ended port.

Use [SetSBPorts Method](#) to set the port mapping for a Single-Ended - Balanced topology.

**VB Syntax** `var = balTopology.SB_SEPort`

**Variable (Type) - Description**

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `variable = balTopology.SB_SEPort 'Read`

**C++ Syntax** HRESULT get\_SB\_SEPort(long \*bVal)

**Interface** IBalancedTopology

## SBalMeasurement Property

---

**Description** Sets and returns the measurement for the Single-Ended - Balanced topology.

**VB Syntax** *balMeas*.**SBalMeasurement** = *value*

**Variable** **(Type) - Description**

*balMeas* A BalancedMeasurement (**object**)

*value* **(String)** - Single-ended - Balanced Measurement parameter. Not case-sensitive. Choose from:

|       |                        |                        |
|-------|------------------------|------------------------|
| Sss11 | Ssd12                  | Ssc12                  |
| Sds21 | Sdd22                  | Sdc22                  |
| Scs21 | Scd22                  | Sc22                   |
| Imb   | CMRR1<br>(Sds21/Scs21) | CMRR2<br>(Ssd12/Ssc12) |

**Return Type** Sss11

**Default** Not Applicable

**Examples**

```
balMeas.SBalMeasurement = "Ssd12" 'Write
variable = balMeas.SBalMeasurement 'Read
```

**C++ Syntax** HRESULT get\_SBalMeasurement(BSTR \*pVal)  
HRESULT put\_SBalMeasurement(BSTR newVal)

**Interface** IBalancedMeasurement

Write/Read.

## Scope Property

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Sets or returns the scope of a trigger signal. This determines whether a trigger signal affects a single channel or all channels in the PNA.<br><hr/> <b>Note:</b> naGlobalTrigger is not compatible with TriggerMode = naTriggerModePoint. If you set Scope = naGlobalTrigger, any channel in naTriggerModePoint will be set to naTriggerModeMeasurement .                    |
| <b>VB Syntax</b>   | <i>trigsetup.Scope = value</i>                                                                                                                                                                                                                                                                                                                                                 |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                    |
| <i>trigsetup</i>   | A <u>TriggerSetup</u> ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                        |
| <i>value</i>       | <b>(enum NATriggerType)</b> - Trigger type. Choose from:<br><b>0 - naGlobalTrigger</b> - a trigger signal is applied to all triggerable channels<br><b>1 - naChannelTrigger</b> - a trigger signal is applied to the current channel. The next trigger signal will be applied to the next channel;not necessarily the next channel in numeric sequence (1-2-3-4 and so forth). |
| <b>Return Type</b> | Long Integer                                                                                                                                                                                                                                                                                                                                                                   |
| <b>Default</b>     | naGlobalTrigger                                                                                                                                                                                                                                                                                                                                                                |
| <b>Examples</b>    | <pre>trigsetup.Scope = naGlobalTrigger 'Write</pre><br><pre>trigtyp = trigsetup.Scope 'Read</pre>                                                                                                                                                                                                                                                                              |
| <b>C++ Syntax</b>  | HRESULT get_Scope(tagNATriggerType *pTrigger)<br>HRESULT put_Scope(tagNATriggerType trigger)                                                                                                                                                                                                                                                                                   |
| <b>Interface</b>   | ITriggerSetup                                                                                                                                                                                                                                                                                                                                                                  |

## SearchFunction Property

---

**Description** Emulates the Tracking function in the marker search dialog box. The value you choose for SearchFunction will determine the type of search that takes place when the Tracking property is set true.

The tracking function finds the selected search function every sweep. In effect, turning Tracking ON is the same as executing one of the "Search..." methods (such as SearchMin, SearchMax) for every sweep.

**VB Syntax** *mark.SearchFunction = value*

**Variable** **(Type) - Description**

*mark* A Marker (**object**)

*value* (**enum NAMarkerFunction**) - search function. Choose from:

- 0** - naMarkerFunction\_ **None**
- 1** - naMarkerFunction\_ **Min**
- 2** - naMarkerFunction\_ **Max**
- 3** - naMarkerFunction\_ **Target**
- 4** - naMarkerFunction\_ **NextPeak**
- 5** - naMarkerFunction\_ **PeakRight**
- 6** - naMarkerFunction\_ **PeakLeft**

**Return Type** Long Integer

**Default** **0** - naMarkerFunction\_ **None**

**Examples** `mark.SearchFunction = naMarkerFunction_Target 'When this marker is set to track, it will track the Target value.`

`searchfunction = mark.SearchFunction 'Read`

**C++ Syntax** HRESULT get\_SearchFunction(tagNAMarkerFunction \*pVal)  
 HRESULT put\_SearchFunction(tagNAMarkerFunction newVal)

**Interface** IMarker



## SecurityLevel Property

---

**Description** Controls the display of frequency information on the PNA screen and printouts.

**VB Syntax** `app.SecurityLevel value`

**Variable** **(Type) - Description**

*app* An Application (**object**)

*value* (**enum NAsSecurityLevel**) -Choose either:

**0 - None** - ALL frequency information is displayed

**1 - Low** - NO frequency information is displayed. Frequency information can be redisplayed using the Security Setting dialog box or this command..

**2- High** - NO frequency information is displayed. Frequency information can be redisplayed ONLY by performing a Preset or recalling an instrument state with None or Low security settings, or using this command.

**Return Type** Long Integer

**Default** 0 - None

**Examples** `app.SecurityLevel = None 'Write`

`level = app.SecurityLevel 'Read`

**C++ Syntax** HRESULT get\_NAsSecurityLevel(tagNAsSecurityLevel \*level);  
HRESULT put\_NAsSecurityLevel(tagNAsSecurityLevel level);

**Interface** IApplication4

## SegmentNumber Property

---

**Description** Returns the number of the current segment, PowerSensorCalFactorSegment or PowerLossSegment object.

**VB Syntax** `seg.SegmentNumber`

**Variable** **(Type) - Description**

`seg` **(object)** - A Segment, PowerSensorCalFactorSegment or PowerLossSegment. Get a handle to the object by referring to the item in the appropriate collection (Segments, CalFactorSegments or PowerLossSegments).

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `segNum = seg.SegmentNumber 'returns the segment number -Read`

**C++ Syntax** HRESULT get\_SegmentNumber(long \*pVal)

**Interface** ISegment  
IPowerSensorCalFactorSegment  
IPowerLossSegment

## ShowStatistics Property

---

**Description** Displays and hides the measurement (Trace) statistics (peak-to-peak, mean, standard deviation) on the screen. To display measurement statistics for a narrower band of the X-axis, use [StatisticsRange](#).

The analyzer will display either measurement statistics or Filter Bandwidth statistics; not both.

**VB Syntax** *meas.ShowStatistics = value*

**Variable (Type) - Description**

*meas* A Measurement (**object**)

*value* (**boolean**) - Boolean value:

**1** - Show statistics

**0** - Hide statistics

**Return Type** Boolean

**Default** 0 - Hide

**Examples** `meas.ShowStatistics = True 'Write`

`showstats = meas.ShowStatistics 'Read`

**C++ Syntax** HRESULT put\_ShowStatistics(VARIANT\_BOOL bState)

**Interface** IMeasurement

## ShowProperties Property

---

**Description** Turns ON and OFF the display of the current switch states on the specified E5091A.

**VB Syntax** *testsets(1).ShowProperties = value*

**Variable** **(Type) - Description**

*testsets(1)* An item from Testsets (**collection**)  
Learn how to identify a testset in the collection.

*value* **(Boolean)**

**ON(1)** Turns display of testset properties ON.

**OFF (0)** Turns display of testset properties OFF.

**Return Type** Boolean

**Default** OFF

**Examples** [See Example Program](#)

**C++ Syntax** HRESULT get\_ShowProperties(VARIANT\_BOOL \*state);  
HRESULT put\_ShowProperties(VARIANT\_BOOL state);

**Interface** IE5091Testsets

## SICL Property

---

**Description** Allows you to control the PNA via SICL (standard instrument control library). In this mode, the analyzer can receive SCPI commands from the LAN interface or from a program residing on the PNA itself. This command performs the same function as the SICL / GPIB dialog box - **SICL Enabled** checkbox. See Configuring the analyzer for SICL/VISA.

With this method you can augment a test program written using SICL that resides on the PNA so that it will run unattended. An automation script can be written to start the PNA, enable SICL (using the SICL property), and then start the SICL based program.

**VB Syntax** *app.SICL value*

**Variable** **(Type) - Description**

*app* An Application (**object**)

*value* (**Boolean**) Choose from:

True - enable SICL

False - disable SICL

**Return Type** Boolean

**Default** False

**Examples**

```
Dim Pna as AgilentPNA835x.Application
Dim siclState as Boolean
Set Pna = CreateObject("AgilentPNA835x.Application")
Pna.SICL = true 'write
```

```
siclState = Pna.SICL 'Read
```

**C++ Syntax** HRESULT get\_SICL(VARIANT\_BOOL \*pVal)  
 HRESULT put\_SICL(VARIANT\_BOOL newVal)

**Interface** IApplication5

## SICLAddress Property

---

**Description** Sets and returns the PNA SICL address. This is the address used for SICL over LAN.

**VB Syntax** `app.SICLAddress = value`

**Variable** (Type) - Description

*app* An Application (**object**)

*value* (Integer) SICL Address of the PNA. Choose a value between 0 and 30.

**Return Type** Short Integer

**Default** 16

**Examples** `address=app.SICLAddress 'Read`

`app.SICLAddress=16 'Write`

**C++ Syntax** `HRESULT get_SICLAddress(short busIndex, short* address);`  
`HRESULT put_SICLAddress(short busIndex,short address);`

**Interface** IApplication8

## Simultaneous2PortAcquisition Property

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p>Specifies whether a 2-port calibration will be done with a single set of standards (one port at a time) or with two sets of standards (simultaneously).</p> <p>The <code>AcquireCalStandard2</code> command uses the same standard index for each calibration class. To specify the calibration standard gender for each port, you must first ensure that the order of calibration class accurately reflects the configuration of your DUT. For example, for a DUT with a male connector on port 1 and a female connector on port 2, order the devices within the S11 classes (A, B, and C) such that the MALE standards are first in the list. Then order the S22 classes specifying the FEMALE standards as the first in the list.</p> |
| <b>VB Syntax</b>   | <code>cal.Simultaneous2PortAcquisition = state</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <code>cal</code>   | A Calibrator ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <code>state</code> | <b>(boolean)</b> - Choose from:<br><b>True</b> - measures 2 ports simultaneously<br><b>False</b> - measures 1 port at a time                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Return Type</b> | Boolean                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>Default</b>     | False                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Examples</b>    | <code>cal.Simultaneous2PortAcquisition = True</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| <b>C++ Syntax</b>  | <code>HRESULT put_Simultaneous2PortAcquisition( VARIANT_BOOL bTwoSetsOfStandards)</code><br><code>HRESULT Simultaneous2PortAcquisition( VARIANT_BOOL *bTwoSetsOfStandards)</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Interface</b>   | ICalibrator                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |

Write/Read

## SmoothingAperture Property

---

**Description** Specifies or returns the amount of smoothing as a ratio of the number of data points in the measurement trace.

**VB Syntax** `meas.SmoothingAperture = value`

**Variable (Type) - Description**

`meas` A Measurement (**object**)

`value` (**double**) - Smoothing Aperture. A ratio of (aperture points / trace points)/100 Choose any number between **.01** and **.25**.

**Return Type** Double

**Default** .25

**Examples**

```
meas.SmoothingAperture = .10 'Write
saperture = meas.SmoothingAperture 'Read
```

**C++ Syntax** HRESULT get\_SmoothingAperture(double \*pVal)  
 HRESULT put\_SmoothingAperture(double newVal)

**Interface** IMeasurement



## Smoothing Property

---

**Description** Turns ON and OFF data smoothing.

**VB Syntax** `meas.Smoothing = state`

**Variable** (Type) - Description

`meas` A Measurement (**object**)

`state` (**boolean**)  
1 - Turns smoothing ON  
0 - Turns smoothing OFF

**Return Type** Boolean

**Default** 0

**Examples** `meas.Smoothing = 1 'Write`

`smooth = meas.Smoothing 'Read`

**C++ Syntax** HRESULT get\_Smoothing(VARIANT\_BOOL \*pVal)  
HRESULT put\_Smoothing(VARIANT\_BOOL newVal)

**Interface** IMeasurement

Write/Read

**SnPFormat Property**

---

**Description** Specifies the format of .S1P, .S2P, .S3P data.Use either app.Save (saves data to file) or meas.GetSnPData (reads data into variant array).**VB Syntax** *pref.SnPFormat = value***Variable** **(Type) - Description***pref* A Preferences (**object**)*value* (**string**) - Format of the .S1P, .S2P, .S3P data. Choose from:**"MA"** - Linear Magnitude / degrees**"DB"** - Log Mag / degrees**"RI"** - Real / Imaginary**"Auto"** - Format in which the trace is already displayed. If other than Log Mag, Linear Magnitude, or Real/Imag, then the format will be in Real/Imag.**Return Type** String**Default** "Auto"**Examples** `pref.SnPFormat = "MA" 'Write``format = pref.SnPFormat 'Read`**C++ Syntax** HRESULT get\_SnPFormat(BSTR \*Format)  
HRESULT put\_SnPFormat(BSTR Format)**Interface** IPreferences

Write/Read

**SoundOnFail Property**

---

**Description** Turns ON or OFF the audio indicator for limit failures.**VB Syntax** *limitst.SoundOnFail = state***Variable** **(Type) - Description***limitst* A LimitTest **(object)***state* **(boolean)**  
0 - Turns the sound OFF  
1 - Turns the sound ON**Return Type** Long Integer**Default** 1 - ON**Examples** `Limttest.SoundOnFail = 1 'Write``sound = Limttest.SoundOnFail 'Read`**C++ Syntax** HRESULT get\_SoundOnFail(VARIANT\_BOOL \*pVal)  
HRESULT put\_SoundOnFail(VARIANT\_BOOL newVal)**Interface** ILimitTest

## SourceCount Property

---

**Description** Returns the number of sources in the remote PNA.

**VB Syntax** *value* = *cap*.SourceCount

**Variable** (Type) - Description

*value* (Long) - Variable to store the returned number of sources.

*cap* A [Capabilities](#) (object)

**Return Type** Long

**Default** Not Applicable

**Examples** `value = cap.SourceCount 'Read`

**C++ Syntax** HRESULT get\_SourceCount(long \* sourceCount );

**Interface** ICapabilities

Read-only

## SourcePort Property

---

**Description** Returns the source port of measurement. To understand how this property is useful, see [IMeasurement2 Interface](#).

**VB Syntax** `value = meas.SourcePort`

**Variable** **(Type) - Description**

`meas` A Measurement **(object)**

`value` **(Long)** - Variable to store the returned value

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `sp = meas.SourcePort`

**C++ Syntax** HRESULT SourcePort( [out, retval] Long\* srcPort);

**Interface** IMeasurement2

Write/Read

**Source Property**

---

**Description** Sets or returns the source of triggering in the PNA.**VB Syntax** *trigSetup.Source* = *value***Variable (Type) - Description***trigSetup* A [TriggerSetup](#) (object)*value* (enum **NATriggerSource**) - Choose from:**0 - naTriggerSourceInternal** - free run**1 - naTriggerSourceManual** - manual trigger source; use app.[ManualTrigger](#) to send a trigger signal.**2 - naTriggerSourceExternal** - a trigger signal is generated when a trigger signal is sensed on the [external trigger pin](#) of the Aux IO connector. Use [ExternalTriggerConnectionBehavior](#) to configure the characteristics of the external trigger signal.**Return Type** Long Integer**Default** naTriggerSourceInternal**Examples**

```
trigSetup.Source = naTriggerSourceInternal 'Write
```

```
trigsource = trigSetup.Source 'Read
```

**C++ Syntax** HRESULT get\_Source(tagNATriggerSource \*pTrigger);  
HRESULT put\_Source(tagNATriggerSource trigger);**Interface** ITriggerSetup

## SourcePowerCalPowerOffset Property

---

**Description** Sets or returns a power level offset from the PNA test port power. This can be a gain or loss value (in dB) to account for components you connect between the source and the reference plane of your measurement. For example, specify 10 dB to account for a 10 dB amplifier at the input of your DUT.

Cal power is the sum of the test port power setting and this offset value. Following the calibration, the PNA power readouts are adjusted to the cal power.

This property performs the same function as the power offset argument on the [SetCallInfo2 Method](#)

**VB Syntax** `chan.SourcePowerCalPowerOffset (sourcePort) = value`

**Variable** **(Type) - Description**

`chan` **(object)** - A [Channel](#) object

`sourcePort` **(long integer)** - The source port for which to set this power offset value.

`value` **(double)** - Gain or loss value in dB. Choose a value between -200 and 200

**Return Type** Double

**Default** 0 dB

**Examples**

```
chan.SourcePowerCalPowerOffset(1) = 10 'Write
offset = chan.SourcePowerCalPowerOffset(2) 'Read
```

**C++ Syntax** HRESULT get\_SourcePowerCalPowerOffset(long sourcePort, double \*pVal);  
HRESULT put\_SourcePowerCalPowerOffset(long sourcePort, double newVal);

**Interface** IChannel4

## SourcePowerCorrection Property

---

**Description** Sets source power correction ON or OFF for a specific source port on this channel, or returns the current ON or OFF state of correction for that source port.

**VB Syntax** `chan.SourcePowerCorrection(sourcePort) = value`

**Variable** **(Type) - Description**

*chan* **(object)** – A Channel object

*sourcePort* **(long integer)** – Source port for which to set or return the ON or OFF state of source power correction.

*value* **(boolean)**

False (0) – Turns source power correction OFF for the source port.

True (1) – Turns source power correction ON for the source port.

**Return Type** Boolean

**Default** False (0) - Source power correction will turn correction ON

**Examples** `chan.SourcePowerCorrection(1) = 1 'Write  
calOnPort2 = chan.SourcePowerCorrection(2) 'Read`

**C++ Syntax** HRESULT put\_SourcePowerCorrection(VARIANT\_BOOL bState);  
HRESULT get\_SourcePowerCorrection(VARIANT\_BOOL \*bState);

**Interface** IChannel



Write/Read

## SourcePowerOption Property

---

**Description** Enables the source power to be set on individual sweep segments. This property must be set True **before** `seg.TestPortPower = value` is sent. Otherwise, the test port power command will be ignored.

**VB Syntax** `segs.SourcePowerOption = state`

**Variable (Type) - Description**

`segs` A Segments collection (**object**)

`state` (**boolean**)

**True (1)** - Enables variable TestPortPower to be set segment sweep

**False (0)** - Disables variable TestPortPower to be set segment sweep

**Return** Boolean

**Type** True - Enabled

False - Disabled

**Default** False

**Examples** `segs.SourcePowerOption = True 'Write`

`powerOption = SourcePowerOption 'Read`

**C++ Syntax** HRESULT get\_SourcePowerOption(VARIANT\_BOOL \*pVal)  
 HRESULT put\_SourcePowerOption(VARIANT\_BOOL newVal)

**Interface** ISegments

## SourcePowerState Property

---

**Description** Turns Source Power ON and OFF.

[See note about source power state with instrument state save and recall.](#)

**VB Syntax** `app.SourcePowerState = state`

**Variable** **(Type) - Description**

`app` An [Application](#) (**object**)

`state` (**boolean**)

**False (0)** - Turns Source Power OFF

**True (1)** - Turns Source Power ON

**Return Type** Boolean  
**0** - Power OFF  
**1** - Power ON

**Default** ON (1)

**Examples** `app.SourcePowerState = True 'Write`

`pwr = app.SourcePowerState 'Read`

**C++ Syntax** HRESULT get\_SourcePowerState(VARIANT\_BOOL \*pVal)  
HRESULT put\_SourcePowerState(VARIANT\_BOOL newVal)

**Interface** IApplication

Write/Read

**Span Property**

---

|                    |                                                                                                                                                                                            |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Sets or returns the Span time of either Gating or Time Domain transform windows                                                                                                            |
| <b>VB Syntax</b>   | <i>object</i> . <b>Span</b> = <i>value</i>                                                                                                                                                 |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                |
| <i>object</i>      | <b>(object)</b> As Gating<br>or<br><b>(object)</b> As Transform                                                                                                                            |
| <i>value</i>       | <b>(double)</b> - Span time in seconds. Choose any number between: <b>2*[(number of points-1) / frequency span]</b> and <b>0</b>                                                           |
| <b>Return Type</b> | Double                                                                                                                                                                                     |
| <b>Default</b>     | 20ns                                                                                                                                                                                       |
| <b>Examples</b>    | <pre>Trans.Span = 4.5e-9 'sets the time span of a transform window -<br/>Write<br/>Gate.Span = 4.5e-9 'sets the Span time of a gating window -Write<br/><br/>span = Trans.Span 'Read</pre> |
| <b>C++ Syntax</b>  | HRESULT get_Span(double *pVal)<br>HRESULT put_Span(double newVal)                                                                                                                          |
| <b>Interface</b>   | ITransform<br>IGating                                                                                                                                                                      |

Read-only

## Span Property

---

**Description** Returns the stimulus span of the measurement (stop-start data points). To understand how this property is useful, see [IMeasurement2 Interface](#).

**VB Syntax** `value = meas.Span`

**Variable** **(Type) - Description**

`value` **(Double)** - Variable to store the returned value.

`meas` A Measurement **(object)**

**Return Type** Double

**Default** Not Applicable

**Examples** `Print meas.Span 'prints the span of the measurement`

**C++ Syntax** `HRESULT get_Span(double * Val);`

**Interface** IMeasurement2

## SSB\_BalPortNegative Property

---

**Description** With a Single-ended - Single-ended - Balanced topology, returns the PNA port number that is connected to the Negative side of the DUT's Balanced Port.

Use [SetSSBPorts Method](#) to set the port mapping for a Single-Ended - Single-Ended - Balanced topology.

**VB Syntax** `var = balTopology.SSB_BalPortNegative`

**Variable (Type) - Description**

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `variable = balTopology.SSB_BalPortNegative 'Read`

**C++ Syntax** HRESULT get\_SSB\_BalPortNegative(long \*bVal)

**Interface** IBalancedTopology

## SSB\_BalPortPositive Property

---

**Description** With a Single-ended - Single-ended - Balanced topology, returns the PNA port number that is connected to the Positive side of the DUT's Balanced Port.

Use [SetSSBPorts Method](#) to set the port mapping for a Single-Ended - Single-Ended - Balanced topology.

**VB Syntax** `var = balTopology.SSB_BalPortPositive`

**Variable (Type) - Description**

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `variable = balTopology.SSB_BalPortPositive 'Read`

**C++ Syntax** HRESULT get\_SSB\_BalPortPositive(long \*bVal)

**Interface** IBalancedTopology

## SSB\_SEPort1 Property

---

**Description** With a Single-ended - Single-ended - Balanced topology, returns the PNA port number that is connected to the DUT's Logical Port 1.

Use [SetSSBPorts Method](#) to set the port mapping for a Single-Ended - Single-Ended - Balanced topology.

**VB Syntax** `var = balTopology.SSB_SEPort1`

**Variable (Type) - Description**

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `variable = balTopology.SSB_SEPort1 'Read`

**C++ Syntax** HRESULT get\_SSB\_SEPort1(long \*bVal)

**Interface** IBalancedTopology

## SSB\_SEPort2 Property

---

**Description** With a Single-ended - Single-ended - Balanced topology, returns the PNA port number that is connected to the DUT's Logical Port 2.

Use [SetSSBPorts Method](#) to set the port mapping for a Single-Ended - Single-Ended - Balanced topology.

**VB Syntax** `var = balTopology.SSB_SEPort2`

**Variable (Type) - Description**

`var` (Long Integer) Variable to store the returned value.

`balTopology` A [BalancedTopology](#) (**object**)

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `variable = balTopology.SSB_SEPort2 'Read`

**C++ Syntax** HRESULT get\_SSB\_SEPort2(long \*bVal)

**Interface** IBalancedTopology



## SSBMeasurement Property

---

**Description** Sets and returns the measurement for the Single-Ended - Single-Ended - Balanced topology.

**VB Syntax** *balMeas*.SSBMeasurement = *value*

**Variable** (Type) - Description

*balMeas* A BalancedMeasurement (**object**)

*value* **(String)** - Single-ended - Single-ended - Balanced Measurement parameter. Not case sensitive. Choose from:

|       |       |                        |                        |
|-------|-------|------------------------|------------------------|
| Sss11 | Sss12 | Ssd13                  | Ssc13                  |
| Sss21 | Sss22 | Ssd23                  | Ssc23                  |
| Sds31 | Sds32 | Sdd33                  | Sdc33                  |
| Scs31 | Scs32 | Scd33                  | Sc33                   |
| lmb1  | lmb2  | CMRR1<br>(Sds31/Scs31) | CMRR2<br>(Sds32/Scs32) |

**Return Type** String

**Default** Sss11

**Examples** `balMeas.SSBMeasurement = "Sss11" 'Write`

`variable = balMeas.SSBMeasurement 'Read`

**C++ Syntax** HRESULT get\_SSBMeasurement(BSTR \*pVal)  
HRESULT put\_SSBMeasurement(BSTR p newVal)

**Interface** IBalancedMeasurement

## StandardDeviation Property

---

**Description** Returns the standard deviation of the measurement.  
To retrieve all 3 statistics value at the same time, use [meas.GetTraceStatistics](#)

**VB Syntax** `stdev = meas.StandardDeviation`

**Variable** (Type) - Description

`stdev` **(single)** - Variable to store standard deviation value

`meas` A Measurement **(object)**

**Return Type** Single

**Default** Not applicable

**Examples** `stdev = meas.StandardDeviation 'Read`

**C++ Syntax** HRESULT get\_StandardDeviation(float\* stdDeviation)

**Interface** IMeasurement

## StandardForClass Property - OBSOLETE

---

**Description** **Obsolete** This command sets a **single** standard to a calibration class. Does NOT set or dictate the order for measuring the standards.

Use [GetStandardForClass](#) and [SetStandardForClass](#). These commands allow up to seven standards to be assigned to a cal class.

**VB Syntax** *calKit*.**StandardForClass**(*class*, *portNum*) = *value*

**Variable** **(Type) - Description**

*calKit* A CalKit (**object**). Use *calKit*.[GetCalStandard](#) to get a handle to the standard.

*class* (**enum NACalClass**) Standard. Choose from:

- 1 - naClassA
- 2 - naClassB
- 3 - naClassC
- 4 - naClassD
- 5 - naClassE
- 6 - naReferenceRatioLine
- 7 - naReferenceRatioThru

### SOLT Standards

- 1 - naSOLT\_Open
- 2 - naSOLT\_Short
- 3 - naSOLT\_Load
- 4 - naSOLT\_Thru
- 5 - naSOLT\_Isolation

### TRL Standards

- 1 - naTRL\_Reflection
- 2 - naTRL\_Line\_Reflection
- 3 - naTRL\_Line\_Tracking
- 4 - naTRL\_Thru
- 5 - naTRL\_Isolation

*portNum* (**long**) - The port number the standard will be connected to. For example, you may have a 3.5mm connector designated for port 1, and Type N designated for port 2.

*value* (**long**) - Calibration class number. Choose a number between **1** and **8**. The *<value>* numbers are associated with the following calibration classes:

| <b>&lt;value&gt;</b> | <b>Class</b> | <b>Description</b>  |
|----------------------|--------------|---------------------|
| 1                    | S11A         | Reflection standard |
| 2                    | S11B         | Reflection standard |
| 3                    | S11C         | Reflection standard |
| 4                    | S21T         | Thru standard       |
| 5                    | S22A         | Reflection standard |
| 6                    | S22B         | Reflection standard |
| 7                    | S22C         | Reflection standard |
| 8                    | S21T         | Thru standard       |

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `calKit.StandardForClass(naSOLT_Short, 1) = 1`

`Kclass = calKit.StandardForClass(naSOLT_Short, 1)`

**C++ Syntax** HRESULT put\_StandardForClass (NACalClass item, long pNum);  
 HRESULT get\_StandardForClass (NACalClass\* item, long \*pNum);

**Interface** ICalKit

Write/Read

### StartFrequency Property

---

**Description** Sets or returns the start frequency of the channel  
**or**  
Sets or returns the start frequency of the segment.  
see also Measurement2 interface

**VB Syntax** *object*.StartFrequency = *value*

**Variable** (Type) - Description

*object* Channel (**object**)  
**or**  
CalSet (**object**) - Read-only property

*value* (**double**) - Start frequency in Hertz. Choose any number between the **minimum** and **maximum** frequencies of the analyzer.

**Return Type** Double

**Default** Channel - Minimum frequency of the analyzer  
Segment - 0

**Examples** `chan.StartFrequency = 4.5e9 'sets the start frequency of a linear sweep for the channel object -Write`

`startfreq = Chan.StartFrequency 'Read`

**C++ Syntax** HRESULT get\_StartFrequency(double \*pVal)  
HRESULT put\_StartFrequency(double newVal)

**Interface** IChannel  
ISegment  
|CalSet3

## StartPower Property

---

**Description** Sets the start power of the analyzer when sweep type is set to Power Sweep. Frequency of the measurement is set with `chan.CWFrequency`.

**VB Syntax** `object.StartPower = value`

**Variable** **(Type) - Description**

*object* Channel (**object**)

**or**

CalSet (**object**) - Read-only property

*value* (**double**) - Start Power in dBm.

---

**Note:** The range of settable power values depends on the PNA model and if source attenuators are installed. To determine the range of values, use `cap.MaximumSourceALCPower` and `cap.MinimumSourceALCPower`

---

Auto attenuation is not allowed in Power Sweep.

**Return Type** Double

**Default** 0

**Examples** `Chan.StartPower = -10 'Write`

```
strtpwr = Chan.StartPower 'Read
```

**C++ Syntax** HRESULT get\_StartPower(double \*pVal)  
HRESULT put\_StartPower(double newVal)

**Interface** IChannel  
|CalSet3

Write/Read

**Start Property**

---

**Description** Sets or returns the start time of either Gating or Time Domain transform windows**VB Syntax** *object*.**Start** = *value***Variable** **(Type) - Description***object* **(object)** As Gating  
**or**  
**(object)** As Transform*value* **(double)** - Start time in seconds. Choose any number between:  
**± (number of points-1) / frequency span****Return Type** Double**Default** -10ns**Examples**  

```
Trans.Start = 4.5e-9 'sets the start time of a transform window
-Write
Gate.Start = 4.5e-9 'sets the start time of a gating window -
Write
```

```
strt = Trans.Start 'Read
```

**C++ Syntax** HRESULT get\_Start(double \*pVal)  
HRESULT put\_Start(double newVal)**Interface** ITransform  
IGating

Read-only

## Start Property

---

**Description** Returns the stimulus value of the first data point for the measurement. To understand how this property is useful, see [IMeasurement2 Interface](#).

**VB Syntax** `value = meas.Start`

**Variable** **(Type) - Description**

`value` **(Double)** - Variable to store the returned value

`meas` A Measurement **(object)**

**Return Type** Double

**Default** Not Applicable

**Examples** `Print meas.Start` 'prints the stimulus value of the first data point

**C++ Syntax** HRESULT get\_Start (double \* Val);

**Interface** IMeasurement2



## State Property

---

**Description** Turns an Object ON and OFF.

**VB Syntax** *object.State* = *value*

**Variable** **(Type) - Description**

*object* Applies to any of the following:  
 Gating (object)  
 InterfaceControl (object)  
 LimitTest (object)  
 Port Extension (object) - OBSOLETE ([See Fixturing Object](#))  
 Segment (object)  
 Transform (object)

---

**Note:** For LimitTest.State - If using Global Pass/Fail status, trigger the PNA AFTER turning Limit testing ON.

---

*value* **(boolean)** -  
**0** - Turns *obj* OFF  
**1** - Turns *obj* ON

**Return Type** Long Integer

**Default** Depends on the object:  
**0** - Gating  
**0** - InterfaceControl  
**0** - LimitTest  
**0** - Port Extension  
**1** - Segment  
**0** - Transform

**Examples** `Seg.State = 1 'Turns the segment object ON -Write`

`tran = Trans.State 'returns the state of Transform -Read`

**C++ Syntax** HRESULT get\_State(VARIANT\_BOOL \*pVal)  
 HRESULT put\_State(VARIANT\_BOOL newVal)

**Interface** ISegment  
 IInterfaceControl  
 ITransform  
 IGating  
 ILimitTest  
 IPortExtension

Write/Read

## Statistics Range Property

---

**Description** Sets the User Range number for calculating measurement statistics. Set the start and stop values for a User Range with `chan.UserRangeMin` and `chan.UserRangeMax`.

There are 16 User Ranges per channel. User ranges are applied independently to any measurement.

**VB Syntax** `meas.StatisticsRange = value`

**Variable** (Type) - Description

`meas` A Measurement **(object)**

`value` **(long integer)** - Range Number. Choose any number between 0 and 16

**0** is Full Span

**1 - 16** are user-defined ranges

**Return Type** Long Integer

**Default** 0

**Examples** `meas.StatisticsRange = 2 'Write`

`statrange = meas.StatisticsRange 'Read`

**C++ Syntax** HRESULT get\_StatisticsRange(long\* rangeNumber)  
 HRESULT put\_StatisticsRange(long rangeNumber)

**Interface** IMeasurement

Write/Read

## StepRiseTime Property

---

**Description** Sets or returns the Rise time of the stimulus in Low Pass Step Mode.

**VB Syntax** *trans*.StepRiseTime = *value*

**Variable** (Type) - Description

*trans* A Transform (**object**)

*value* (**double**) - Rise time in seconds. Choose any number between **5.0e-13** and **1.63e-14**.

**Return Type** Double

**Default** 0

**Examples** `trans.StepRiseTime = 1.0e-14 'sets the step rise time to 100 psec. -Write`

`rt = trans.StepRiseTime 'Read`

**C++ Syntax** HRESULT get\_StepRiseTime(double \*pVal)  
HRESULT put\_StepRiseTime(double newVal)

**Interface** ITransform

## StimulusValues Property

---

**Description** Returns multiple X-axis frequency arrays (source and response) needed by frequency offset measurements. The arrays contain one frequency value for each data point.

**VB Syntax** *value* = *object*.**StimulusValues** (*range*)

**Variable** (Type) - Description

*object* Channel (**object**)

**or**

CalSet (**object**) - Read-only property

*range* (**Long**) –

Specify **0** to return source frequencies.

Specify **1** to return response frequencies.

**Return Type** 1-dimensional variant array

**Default** Not Applicable

**Examples** `array = CalSet.StimulusValues 'Read`

**C++ Syntax** HRESULT get\_StimulusValues (long range, VARIANT\* vals)

**Interface** ICalSet3

Write/Read

### StopFrequency Property

---

**Description** Sets or returns the stop frequency of the channel  
**or**  
Sets or returns the stop frequency of the segment.  
see also Measurement2 interface

**VB Syntax** *object*.StopFrequency = *value*

**Variable** (Type) - Description

*object* Channel (**object**)  
**or**  
CalSet (**object**) - Read-only property

*value* (**double**) - Stop frequency in Hertz. Choose any number between the **minimum** and **maximum** frequencies of the analyzer.

**Return Type** Double

**Default** Channel - Maximum frequency of the analyzer  
Segment - 0

**Examples** `chan.StopFrequency = 4.5e9 'sets the stop frequency of a linear sweep for the channel object -Write`

`stopfreq = Chan.StopFrequency 'Read`

**C++ Syntax** HRESULT get\_StopFrequency(double \*pVal)  
HRESULT put\_StopFrequency(double newVal)

**Interface** IChannel  
ISegment  
|CalSet3

## StopPower Property

---

**Description** Sets the Stop Power of the analyzer when sweep type is set to Power Sweep. Frequency of the measurement is set with `chan.CWFrequency`

**VB Syntax** `object.StopPower = value`

**Variable** **(Type) - Description**

*object* Channel (**object**)

**or**

CalSet (**object**) - Read-only property

*value* **(double)** - Stop Power in dB. Start Power in dB.

---

**Note:** The range of settable power values depends on the PNA model and if source attenuators are installed. To determine the range of values, use `cap.MaximumSourceALCPower` and `cap.MinimumSourceALCPower`

---

Auto attenuation is not allowed in Power Sweep.

**Return Type** Double

**Default** 0

**Examples** `Chan.StopPower = -10 'Write`

`stppwr = Chan.StopPower 'Read`

**C++ Syntax** HRESULT get\_StopPower(double \*pVal)  
HRESULT put\_StopPower(double newVal)

**Interface** IChannel  
|CalSet3

Write/Read

**Stop Property**

---

**Description** Sets or returns the Stop time of either Gating or Time Domain transform windows**VB Syntax** *object*.**Stop** = *value***Variable** **(Type) - Description***object* **(object)** As Gating  
or  
**(object)** As Transform*value* **(double)** - Start time in seconds. Choose any number between:  
**± (number of points-1) / frequency span****Return Type** Double**Default** 10 ns**Examples**  

```
Trans.Stop = 4.5e-9 'sets the stop time of a transform window -
Write
Gate.Stop = 4.5e-9 'sets the stop time of a gating window -Write

stp = Trans.Stop 'Read
```

**C++ Syntax** HRESULT get\_Stop(double \*pVal)  
HRESULT put\_Stop(double newVal)**Interface** ITransform  
IGating

Read- only

## Stop Property

---

**Description** Returns the stimulus value of the last data point for the measurement. To understand how this property is useful, see [IMeasurement2 Interface](#).

**VB Syntax** *value* = *meas*.**Stop**

**Variable** (Type) - Description

*value* **(Double)** Variable to store the returned value

*meas* A Measurement **(object)**

**Return Type** Double

**Default** Not Applicable

**Examples** `Print meas.Stop 'prints the stimulus value of the last data point`

**C++ Syntax** HRESULT get\_Stop(double \* Val);

**Interface** IMeasurement2



## strPort2Pdeembed\_S2PFile Property

---

**Description** Sets and returns the 2 port De-embedding .S2P file name for the specified port number. Model is applied when both the file name is specified and **User** is specified using [Port2PdeembedCktModel Property](#).

[Learn more about S2P files.](#)

---

**Note:** This command affects ALL measurements on the channel.

---

**VB Syntax** `fixture.strPort2Pdeembed_S2PFile(port) = value`

**Variable (Type) - Description**

`fixture` A [Fixturing \(object\)](#)

`port` **(Integer)** Port number to receive circuit model.

`value` **(String)** Full path, file name, and extension (.s2P) of the de-embedding circuit. Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents

**Return Type** String

**Default** Not Applicable

**Examples** `fixture.strPort2Pdeembed_S2PFile(2) = "C:\Program Files\Agilent\Network Analyzer\Documents\myFile.s2p" 'Write`

`value = fixture.strPort2Pdeembed_S2PFile(1) 'Read`

**C++ Syntax** HRESULT get\_strPort2Pdeembed\_S2PFile(short port BSTR \*bstrFile)  
 HRESULT put\_strPort2Pdeembed\_S2PFile(short port BSTR bstrFile)

**Interface** IFixturing

## strPortMatch\_S2PFile Property

---

**Description** Sets and returns the Port Matching 'S2P' file name for the specified port number. Model is applied when both the file name is specified and **User** is specified using [PortMatchingCktModel Property](#).

[Learn more about S2P files.](#)

**Note:** This command affects ALL measurements on the channel.

---

**VB Syntax** *fixture.strPort2PMatch\_S2PFile(port) = value*

**Variable (Type) - Description**

*fixture* A [Fixturing](#) (**object**)

*port* (**Integer**) Port number to receive circuit model.

*value* (**String**) Full path, file name, and extension (.s2P) of the matching circuit. Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents".

**Return Type** String

**Default** Not Applicable

**Examples** `fixture.strPort2PMatch_S2PFile(2) = "C:\Program Files\Agilent\Network Analyzer\Documents\myFile.s2p" 'Write`

`value = fixture.strPort2PMatch_S2PFile(1) 'Read`

**C++ Syntax** HRESULT get\_strPort2PMatch\_S2PFile(short port BSTR \*bstrFile)  
 HRESULT put\_strPort2PMatch\_S2PFile(short port BSTR bstrFile)

**Interface** IFixturing

## SweepEndMode Property

---

**Description** Sets and reads the event that will cause the Sweep End line to go to a low state. The line will return to a high state after the appropriate calculations are complete.

**Note:** This line is connected to the following pins on the HANDLER IO connector and AUX IO connector in the PNA. Therefore, this command will affect both of these connectors in the same way.

---

**VB Syntax** *object*.SweepEndMode = *value*

**Variable** **(Type) - Description**

*object* **(object)** - A HandlerIO or AuxIO object

*value* (enum as NASweepEndMode ) Choose from:

0 - naSweep - the line goes low when each sweep is complete

1 - naChannelSweep - the line goes low when all the sweeps for each channel is complete.

2 - naGlobalSweep - the line goes low when all sweeps for all triggerable channels are complete.

**Return Type** Long Integer

**Default** 0 - naSweep

**Examples**

```
HWAuxIO.PassFailMode = naSweep 'Write
value = HWAuxIO.PassFailMode 'Read
```

**C++ Syntax**

```
HRESULT put_SweepEndMode (tagNASweepEndMode Mode);
HRESULT get_SweepEndMode (tagNASweepEndMode* Mode);
```

**Interface**

```
IHWAuxIO
IHWMaterialHandlerIO
```

## SweepHoldOff Property

---

|                    |                                                                                                                                                 |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Returns a boolean that represents the state of SweepHoldoff line (pin2) of the External Test Set connector.                                     |
| <b>VB Syntax</b>   | <i>value</i> = <i>ExtIO.SweepHoldOff</i>                                                                                                        |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                     |
| <i>value</i>       | <b>(boolean)</b> - Variable to store the returned data                                                                                          |
| <i>ExtIO</i>       | <b>(object)</b> - An External IO object                                                                                                         |
| <b>Return Type</b> | Boolean<br><b>False (0)</b> - indicates the line is being held at a TTL Low<br><b>True (1)</b> - indicates the line is being held at a TTL High |
| <b>Default</b>     | Not Applicable                                                                                                                                  |
| <b>Examples</b>    | <code>value = ExtIO.SweepHoldOff</code>                                                                                                         |
| <b>C++ Syntax</b>  | HRESULT get_SweepHoldOff( VARIANT_BOOL* bValue);                                                                                                |
| <b>Interface</b>   | IHWExternalTestSetIO                                                                                                                            |

## SweepGenerationMode Property

---

**Description** Sets the method used to generate a sweep: continuous ramp (analog) or discrete steps (stepped).

**VB Syntax** *object*.SweepGenerationMode = *value*

**Variable** (Type) - Description

*object* Channel (**object**)

**or**

CalSet (**object**) - Read-only property

*value* (**enum NASweepGenerationModes**) - **Choose either:**

**0 - naSteppedSweep** - source frequency is CONSTANT during measurement of each displayed point. More accurate than Analog. Dwell time can be set in this mode.

**1 - naAnalogSweep** - source frequency is continuously RAMPING during measurement of each displayed point. Faster than Stepped. Sweep time (not dwell time) can be set in this mode.

**Return Type** Long Integer

**Default** Analog

**Examples** `Chan.SweepGenerationMode = naAnalogSweep 'Write`

`swpgen = Chan.SweepGenerationMode 'Read`

**C++ Syntax** HRESULT get\_SweepGenerationMode(tagNASweepGenerationModes\* pVal)  
 HRESULT put\_SweepGenerationMode(tagNASweepGenerationModes newVal)

**Interface** IChannel  
 |CalSet3

## SweepTime Property

---

**Description** Sets the Sweep time of the analyzer. If sweep time accuracy is critical, use ONLY the values that are attained using the up and down arrows next to the sweep time entry box. [See Sweep Time.](#)

**VB Syntax** *object.SweepTime = value*

**Variable** **(Type) - Description**

*object* Channel **(object)**

**or**

CalSet **(object)** - Read-only property

*value* **(double)** - Sweep time in seconds. The maximum sweep time of the PNA is 86400 seconds (1 day).

To set the fastest sweep speed possible, set this value to 0.

**Return Type** Double

**Default** 0

**Examples** `chan.SweepTime = 3e-3 'Write`

`swptme = chan.SweepTime 'Read`

**C++ Syntax** HRESULT get\_SweepTime(double \*pVal)  
HRESULT put\_SweepTime(double newVal)

**Interface** IChannel  
CalSet3

Write/Read

**SweepType Property**

---

**Description** Sets the type of X-axis sweep that is performed on a channel.**VB Syntax** *object*.SweepType = *value***Variable (Type) - Description***object* Channel (**object**)**or**CalSet (**object**) - Read-only property*value* (**enum NASweepTypes**) - Choose from:**0 - naLinearSweep****1 - naLogSweep****2 - naPowerSweep****3 - naCWTimeSweep****4 - naSegmentSweep**

---

**Note:** Sweep type cannot be set to Segment sweep if there are no segments turned ON. A segment is automatically turned ON when a application is created.

---

**Return Type** Long Integer**Default** naLinearSweep**Examples**

```
chan.SweepType = naPowerSweep 'Write
```

```
swptyp = chan.SweepType 'Read
```

**C++ Syntax** HRESULT get\_SweepType(tagNASweepTypes\* pVal)  
HRESULT put\_SweepType(tagNASweepTypes newVal)**Interface** IChannel  
|CalSet3

## SystemImpedanceZ0 Property

---

**Description** Sets and returns the impedance for the analyzer.

**VB Syntax** `app.SystemImpedanceZ0 = value`

**Variable** (Type) - Description

*app* An Application (**object**)

*value* (double) Analyzer Impedance. Choose any number between 0 and 1000 ohms.

**Return Type** Double

**Default** 50

**Examples** `app.SystemImpedanceZ0 = 75 'Write`

`z0 = app.SystemImpedanceZ0 'Read`

**C++ Syntax** HRESULT get\_SystemImpedanceZ0(double dSystemZ0)  
HRESULT put\_SystemImpedanceZ0(double \*pdSystemZ0)

**Interface** IApplication



## SystemName Property

---

**Description** Returns the computer name of the PNA.

**VB Syntax** `name = app.SystemName`

**Variable** (Type) - Description

`name` (String) Variable to store the returned computer name.

`app` An Application (object)

**Return Type** String

**Default** Not Applicable

**Examples** `name = app.SystemName`

**C++ Syntax** HRESULT SystemName(BSTR\* computerName)

**Interface** IApplication

## TargetValue Property

---

**Description** Sets the target value for the marker when doing Target Searches ([SearchTargetLeft](#), [SearchTarget](#), [SearchTargetRight](#)).

**VB Syntax** `mark.TargetValue = value`

**Variable** **(Type) - Description**

`mark` A Marker (**object**)

`value` (**single**) - Target value. Choose any number between: **-500** and **500**

**Return Type** Single

**Default** 0

**Examples** `mark.TargetValue = 10.5 'Write`

`target = mark.TargetValue 'Read`

**C++ Syntax** HRESULT `get_TargetValue(float *pVal)`  
HRESULT `put_TargetValue(float newVal)`

**Interface** IMarker

## TestPortPower Property

---

**Description** Sets or returns the RF power level for the channel  
**or**  
 Sets or returns the RF power level of the segment.

**VB Syntax** *object*.**TestPortPower**(*portNum*) = *value*

**Variable** (Type) - Description

*object* A Channel (**object**) - to set coupled power, use `chan.CouplePorts`. If `CouplePorts = False`, then each port power can be set independently. Otherwise, `chanTestPortPower (1) = value` sets power level at both ports.

**or**

A CalSet (**object**)

**or**

A Segment (**object**)

*portNum* (**long integer**) - Port number of the source power. Choose from **1** or **2**

*value* (**double**) - RF Power in dBm.

---

Note: The range of settable power values depends on the PNA model and if source attenuators are installed. To determine the range of values, use `cap.MaximumSourceALCPower` and `cap.MinimumSourceALCPower`

---

Actual achievable leveled power depends on frequency.

**Return Type** Double

**Default** 0

**Examples** `chan.TestPortPower(1) = 5 'sets the port 1 RF power level for the channel object -Write`

`powerlev = Chan.TestPortPower(1) 'Read`

**C++ Syntax** HRESULT `get_TestPortPower(long port, double *pVal)`  
 HRESULT `put_TestPortPower(long port, double newVal)`

**Interface** IChannel  
 ICalSet3  
 ISegment

## ThruCalMethod Property

---

**Description** Sets and returns the method for performing the thru portion of the calibration.

**VB Syntax** *obj.ThruCalMethod = value*

**Variable** (Type) - Description

*obj* SMCType (object)

or

VMCType (object)

*value* (String) Specifies the Thru method. Case insensitive - include spaces. Choose from:

"Default"

"Flush Thru" **or** "FLUSH"

"Unknown Thru" **or** "UNKN"

"Adapter Removal" **or** "ADAP"

**Return Type** String

**Default** **Default**

**Examples** `SMC.ThruCalMethod = "UNKN"`

**C++ Syntax** HRESULT put\_ThruCalMethod(enum NATHruCalMethod thruMethod);  
 HRESULT get\_ThruCalMethod(enum NATHruCalMethod \*thruMethod);

**Interface** SMCType

VMCType

## ThruCalMethod Property

---

**Description** Sets and returns the method for performing the THRU portion of the calibration.

**VB Syntax** `guidedCal.ThruCalMethod = value`

**Variable** **(Type) - Description**

*guidedCal* [GuidedCalibration](#) (object)

*value* (Enum as NAThruCalMethod) Specifies the THRU method. Choose from:

**0 - naDefaultCalMethod** - allow the PNA to choose the best possible method (from the following) depending on whether the device or ECal module is insertable or non-insertable and given the model number of the PNA. (default selection if omitted.)

**1 - naAdapterRemoval** - Perform Adapter removal calibration.

**2 - naFlushThru** - Perform Flush Thru calibration.

**3 - naDefinedThru** - Perform Defined Thru calibration. If performing an ECal, this is the Thru standard in the ECal module.

**4 - naUnknownThru** - Perform Unknown Thru calibration.

**Return Type** Enum

**Default** 0 - naDefaultCalMethod

**Examples** `guided.ThruCalMethod = naDefinedThru`

**C++ Syntax** `HRESULT get_ThruCalMethod(enum NAThruCalMethod *thruMethod);`  
`HRESULT put_ThruCalMethod(enum NAThruCalMethod thruMethod);`

**Interface** IGuidedCalibration

## ThruPortList Property

---

**Description** **Note:** Available only on PNA releases 5.0 and greater.

Sets and returns the thru connection port pairs for the calibration.

- For 3-port cals, specify at least two pairs.
- For 4-port cals, specify at least three pairs.
- For highest accuracy, specify more than the minimum pairs.
- You can query (not set) the thru port pairs for one and two port calibrations.

Learn more about [Thru method and port pairings](#).

See an example of a [4-port guided calibration using COM](#).

**VB Syntax** `guidedCal.ThruPortList = t1a, t1b, t2a, t2b, t3a, t3b`

**Variable** **(Type) - Description**

`guidedCal` [GuidedCalibration](#) (object)

`t1a, t1b...` **(Variant)** Port numbers in pairs:

t1a, t1b (Thru1 - port A and port B)

t2a, t2b (Thru2 - port A and port B)

t3a, t3b (Thru3 - port A and port B)

**Return Type** **Variant** - Returns comma-separated pairs.

**Default** Not Applicable

**Example** `guided.ThruPortList = 1,2,1,3,1,4`

```
'Sets the following three thru connections for a 4-port
calibration:
```

```
Thru 1 - ports 1 and 2
```

```
Thru 2 - ports 1 and 3
```

```
Thru 3 - ports 1 and 4
```

**C++ Syntax** `HRESULT get_ThruPortList(VARIANT* portList);`

`HRESULT put_ThruPortList(VARIANT portList);`

**Interface** `IGuidedCalibration`

Write/Read

## Title Property

---

**Description** Writes or reads a custom title for the window. Newer entries replace (not append) older entries. Turn the title ON and OFF with TitleState

**VB Syntax** `win.Title = string`

**Variable (Type) - Description**

*win* A NaWindow **(object)**

*string* **(long)** - Title limited to 50 characters.

**Return Type** String

**Default** Null

**Examples** `win.Title = "Hello World" 'Write`

`titl = win.Title 'Read`

**C++ Syntax** HRESULT get\_Title(BSTR \*title)  
HRESULT put\_Title(BSTR title)

**Interface** INAWindow

## TitleState Property

---

**Description** Turns ON and OFF the window title. Write a window title with Title

**VB Syntax** `win.TitleState = state`

**Variable** (Type) - Description

`win` A NaWindow **(object)**

`state` **(boolean)**  
**True (1)** - Title ON  
**False (0)** - Title OFF

**Return Type** Long Integer  
**0** - Title OFF  
**1** - Title ON

**Default** 0 - OFF

**Examples** `win.TitleState = True 'Write`

```
titlestate = win.TitleState 'Read
```

**C++ Syntax** HRESULT get\_TitleState(VARIANT\_BOOL\* bState)  
HRESULT put\_TitleState(VARIANT\_BOOL bState)

**Interface** INAWindow



Write/Read

**TraceMath Property**

---

**Description** Performs math operations on the measurement object and the trace stored in memory. (There MUST be a trace stored in Memory to perform math. See [Meas.DataToMemory](#) method.)

**VB Syntax** `meas.TraceMath = value`

**Variable (Type) - Description**

*meas* A measurement (**object**)

*value* (**enum NAMathOperation**) - Choose from:

**0** - naDataNormal

**1** - naDataMinusMemory

**2** - naDataPlusMemory

**3** - naDataDivMemory

**4** - naDataTimesMemory

**Return Type** NAMathOperation

**Default** Normal (0)

**Examples** `meas.TraceMath = naDataMinusMemory 'Write`

`mathOperation = meas.TraceMath 'Read`

**C++ Syntax** HRESULT get\_TraceMath(tagNAMathOperation\* pMathOp)  
HRESULT put\_TraceMath(tagNAMathOperation mathOp)

**Interface** IMeasurement

## Tracking Property

---

**Description** This property, when on, executes the search function (marker.SearchFunction) every sweep. In effect, turning Tracking ON is the same as executing one of the immediate, one-time, "Search..." methods (such as SearchMin, SearchMax) for every sweep.

**VB Syntax** `mark.Tracking = state`

**Variable (Type) - Description**

`mark` A Marker (**object**)

`state` (**boolean**) - Tracking state. Choose from:  
**ON (1)**  
**OFF (0)**

**Return Type** Boolean  
**0** - Tracking OFF  
**1** - Tracking ON

**Default** 0 - OFF

**Examples** `mark.Tracking = 1 'Write`

`markTracking = mark.Type 'Read`

**C++ Syntax** HRESULT put\_Tracking(VARIANT\_BOOL bOn)  
HRESULT get\_Tracking(VARIANT\_BOOL \* pbOn)

**Interface** IMarker

Write/Read

**Mode Property**

---

**Description** Sets the type of transform.**VB Syntax** *trans.Mode* = *value***Variable** **(Type) - Description***trans* A Transform (**object**)*value* (**enum NATransformMode**) - Choose from:**0** - naTransformBandpassImpulse**1** - naTransformLowpassImpulse**2** - naTransformLowpassStep**Return Type** NATransformMode**Default** **0** - naTransformBandpassImpulse**Examples** `trans.Mode = naTransformLowpassStep 'Write``transmode = trans.Mode 'Read`**C++ Syntax** HRESULT get\_Mode(tagNATransformMode \*pVal)  
HRESULT put\_Mode(tagNATransformMode newVal)**Interface** ITransform

## TriggerDelay Property

---

**Description** Sets and reads the trigger delay for all measurements (GLOBAL). This delay is only applied while in `app.Source = naTriggerSourceExternal` and `trigsetup.Scope = naGlobalTrigger` . After an external trigger is applied, the start of the sweep is delayed for the specified delay value plus any inherent latency.

To apply a trigger delay for a channel only, use [ExternalTriggerDelay Property](#).

**VB Syntax** `app.TriggerDelay = value`

**Variable** **(Type) - Description**

`app` An [Application](#) (**object**)

`value` **Double**- Trigger delay value in seconds. Range is from 0 to 107

**Return Type** Double

**Default** 0

**Examples** `app.TriggerDelay = .003 'Write`

`delay = app.TriggerDelay 'Read`

**C++ Syntax** HRESULT get\_TriggerDelay(double \*delay);  
 HRESULT put\_TriggerDelay(double delay)

**Interface** IApplication

## TriggerOutputEnabled Property

---

**Description** Enables the PNA to send trigger signals out the rear-panel TRIGGER OUT connector. For more information, see [External triggering](#).

**VB Syntax** *trigsetup.TriggerOutputEnabled = boolean*

**Variable** **(Type) - Description**

*trigsetup* A [TriggerSetup2](#) (**object**)

*boolean* Choose from:  
**0 - False** - PNA does NOT send output trigger signals.  
**1 - True** - PNA sends output trigger signals.

**Return Type** Boolean

**Default** False

**Examples**

```
trigsetup.TriggerOutputEnabled = 1 'Write
```

```
atba = trigsetup.TriggerOutputEnabled 'Read
```

**C++ Syntax** HRESULT get\_TriggerOutputEnabled( BOOL \*pVal);  
HRESULT put\_TriggerOutputEnabled( BOOL newVal);

**Interface** ITriggerSetup2

## TriggerMode Property

---

**Description** Each trigger signal will cause either:  
all measurements in the channel to be made **or**  
only a single data point in the channel at a time.

**VB Syntax** `chan.TriggerMode = value`

**Variable** (Type) - Description

*chan* A Channel (**object**)

*value* (**enum NATriggerMode**) - Choose from:

**0 - naTriggerModePoint** - a single data point is measured with each trigger signal the channel receives. Subsequent trigger signals continue to go to the channel in Point mode until the channel measurements are complete.

**1 - naTriggerModeMeasurement** - all measurements in the channel are made with each trigger signal the channel receives.

---

**Note:** Point Mode is not compatible when TriggerType is set to naGlobalTrigger. If you change any channel to TriggerModePoint, TriggerType will be set to naChannelTrigger.

---

**Return Type** Long Integer

**Default** 0 - naTriggerModeMeasurement

**Examples** `chan.TriggerMode = naTriggerModePoint 'Write`

```
trigtyp = chan.TriggerMode 'Read
```

**C++ Syntax** HRESULT get\_TriggerMode (tagNATriggerMode \*pMode)  
HRESULT put\_TriggerMode (tagNATriggerMode newMode)

**Interface** IChannel

Write/Read

**TriggerSignal Property - OBSOLETE**

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This command has been replaced by <a href="#">Source Property</a><br>Sets or returns the trigger source.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>VB Syntax</b>   | <code>app.TriggerSignal = value</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <i>app</i>         | An Application ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <i>value</i>       | <b>(enum NATriggerSignal)</b> - Choose from:<br><b>0 - naTriggerInternal</b> - free run<br><b>1 - naTriggerExternalPositive</b> - a trigger signal is generated when a TTL high is sensed on the <a href="#">external trigger pin</a> of the Aux IO connector<br><b>2 - naTriggerExternalNegative</b> - a trigger signal is generated when a TTL low is sensed on the <a href="#">external trigger pin</a> of the Aux IO connector.<br><b>3 - naTriggerManual</b> - manual trigger source; use <code>app.ManualTrigger</code> to send a trigger signal.<br><b>4 - naTriggerExternalHigh</b> - a trigger signal is generated when a TTL high is sensed on the <a href="#">external trigger pin</a> of the Aux IO connector<br><b>5 - naTriggerExternalLow</b> - a trigger signal is generated when a TTL low is sensed on the <a href="#">external trigger pin</a> of the Aux IO connector |
| <b>Return Type</b> | Long Integer                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Default</b>     | naTriggerInternal                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Examples</b>    | <pre>app.TriggerSignal = naTriggerExternalPositive 'Write</pre><br><pre>trigsig = app.TriggerSignal 'Read</pre>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>C++ Syntax</b>  | HRESULT get_TriggerSignal(tagNATriggerSignal *pSignal)<br>HRESULT put_TriggerSignal(tagNATriggerSignal signal)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <b>Interface</b>   | IApplication                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |

Write/Read.

**TriggerType Property - OBSOLETE**

---

|                    |                                                                                                                                                                                                                                                                                                                                     |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This property has been replaced with <u>Scope</u> Property.<br>Sets or returns the trigger type which determines the scope of a trigger signal.                                                                                                                                                                        |
| <b>VB Syntax</b>   | <i>app.TriggerType</i> = <i>value</i>                                                                                                                                                                                                                                                                                               |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                         |
| <i>app</i>         | An Application ( <b>object</b> )                                                                                                                                                                                                                                                                                                    |
| <i>value</i>       | <b>(enum NATriggerType)</b> - Trigger type. Choose from:<br><b>0 - naGlobalTrigger</b> - a trigger signal is applied to all triggerable channels<br><b>1 - naChannelTrigger</b> - a trigger signal is applied to the current channel. The next trigger signal will be applied to the next channel; not necessarily channel 1-2-3-4. |
| <b>Return Type</b> | Long Integer                                                                                                                                                                                                                                                                                                                        |
| <b>Default</b>     | naGlobalTrigger                                                                                                                                                                                                                                                                                                                     |
| <b>Examples</b>    | <pre>app.TriggerType = naGlobalTrigger 'Write</pre><br><pre>trigtyp = app.TriggerType 'Read</pre>                                                                                                                                                                                                                                   |
| <b>C++ Syntax</b>  | HRESULT get_TriggerType(tagNATriggerType *pTrigger)<br>HRESULT put_TriggerType(tagNATriggerType trigger)                                                                                                                                                                                                                            |
| <b>Interface</b>   | IApplication                                                                                                                                                                                                                                                                                                                        |



## Type (calstd) Property

---

**Description** Sets and Returns the type of calibration standard.

**VB Syntax** `calstd.Type = value`

**Variable** (Type) - Description

*calstd* A CalStandard (**object**). Use calKit.GetCalStandard to get a handle to the standard.

*value* (**enum** NACalStandardType) -Choose from:

**0 - naOpen**

**1 - naShort**

**2 - naLoad**

**3 - naThru**

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `calstd.Type = naOpen 'Write`

`standardtype = calstd.Type 'Read`

**C++ Syntax** HRESULT get\_Type(tagNACalStandardType \*pVal)  
HRESULT put\_Type(tagNACalStandardType newVal)

**Interface** ICalStandard

Write/Read

**TZImag Property**

---

**Description** Sets and Returns the TZImag value (the Imaginary Terminal Impedance value) for the calibration standard. Only applicable when "Type" is set to **naArbitraryImpedance**.

To set the other resistance values, use TZReal

**VB Syntax** *calstd.TZImag = value*

**Variable** **(Type) - Description**

*calstd* A CalStandard **(object)**. Use calKit.GetCalStandard to get a handle to the standard.

*value* **(single)** - Value for TZImag in Ohms

**Return Type** Single

**Default** Not Applicable

**Examples** `calstd.TZImag = 15 'Write the value of TZImag to 15 Ohms`

`imp0 = calstd.TZImag 'Read the value of TZImag`

**C++ Syntax** HRESULT get\_TZImag(float \*pVal);  
HRESULT put\_TZImag(float newVal);

**Interface** ICalStandard2

Write/Read

**TZReal Property**

---

**Description** Sets and Returns the TZReal value (the real Terminal Impedance value) for the calibration standard. Only applicable when "Type" is set to **naArbitraryImpedance**.

To set the other resistance values, use TZImag

**VB Syntax** `calstd.TZReal = value`

**Variable** **(Type) - Description**

`calstd` A CalStandard **(object)**. Use `calKit.GetCalStandard` to get a handle to the standard.

`value` **(single)** - Value for TZReal in Ohms

**Return Type** Single

**Default** Not Applicable

**Examples** `calstd.TZReal = 15 'Write the value of TZReal to 15 Ohms`

`imp0 = calstd.TZReal 'Read the value of TZReal`

**C++ Syntax** `HRESULT get_TZReal(float *pVal);`  
`HRESULT put_TZReal(float newVal);`

**Interface** ICalStandard2

Read-only

## UnusedChannelNumbers Property

---

**Description** Returns an array of channel numbers that are NOT in use. An unused channel has NO measurements subscribed to it.

**VB Syntax** *chanNumbers = chans.UnusedChannelNumbers (NumberOfChannels)*

**Variable** **(Type) - Description**

*chanNumbers* Variable array to store the returned channel numbers

*chans* A Channel collection (**object**)

*NumberOfChannels* **(Long Integer)** Number of channels that you are requesting.

**Return Type** One-dimensional array of long integers. The size of the array is specified by the *NumberOfChannels* parameter.

**Default** Not Applicable

**Examples** `chanNumbers = chans.UnusedChannelNumbers(5)`

**C++ Syntax** HRESULT get\_UnusedChannelNumbers(long numberRequested,VARIANT\* channelNumbers);

**Interface** IChannels2

Read-only

## UsedChannelNumbers Property

---

**Description** Returns an array of channel numbers that are in use. A used channel has at least one measurement subscribed to it

**VB Syntax** *chanNumbers* = *chans*.UsedChannelNumbers

**Variable** **(Type) - Description**

*chanNumbers* Variable array to store the returned channel numbers

*chans* A Channel collection (**object**)

**Return Type** One-dimensional array of long integers

**Default** Not Applicable

**Examples** `chanNumbers = chans.UsedChannelNumbers`

**C++ Syntax** HRESULT get\_UsedChannelNumbers(VARIANT\* channelNumbers);

**Interface** IChannels2

## UsePowerLossSegments Property

---

|                    |                                                                                                                                                                        |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Specifies if subsequent calls to the <a href="#">AcquirePowerReadings</a> method will make use of the loss table (PowerLossSegments).                                  |
| <b>VB Syntax</b>   | <i>pwrCal</i> .UsePowerLossSegments = <i>value</i>                                                                                                                     |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                            |
| <i>pwrCal</i>      | <b>(object)</b> – A SourcePowerCalibrator (object)                                                                                                                     |
| <i>value</i>       | <b>(boolean) -</b><br><b>False (0)</b> – Do not use loss table<br><b>True (1)</b> – Use loss table                                                                     |
| <b>Return Type</b> | Boolean                                                                                                                                                                |
| <b>Default</b>     | False                                                                                                                                                                  |
| <b>Examples</b>    | <pre>Set powerCalibrator = pna.SourcePowerCalibrator powerCalibrator.UsePowerLossSegments = 1 'Write lossTableState = powerCalibrator.UsePowerLossSegments 'Read</pre> |
| <b>C++ Syntax</b>  | HRESULT put_UsePowerLossSegments(VARIANT_BOOL bState);<br>HRESULT get_UsePowerLossSegments(VARIANT_BOOL *bState);                                                      |
| <b>Interface</b>   | ISourcePowerCalibrator                                                                                                                                                 |

Write / Read

**UsePowerSensorFrequencyLimits Property**

---

**Description** Specifies if subsequent calls to the `AcquirePowerReadings` method will observe frequency values of the `MinimumFrequency` and `MaximumFrequency` properties.

**VB Syntax** `pwrCal.UsePowerSensorFrequencyLimits = value`

**Variable (Type) - Description**

`pwrCal` **(object)** – A `SourcePowerCalibrator` (object)

`value` **(boolean)** -

**False (0)** – Do not use power sensor frequency limits. An acquisition will use just one power sensor for the entire sweep, regardless of frequency.

**True (1)** – Use power sensor frequency limits. A requested acquisition will only succeed for those frequency points which fall between the `MinimumFrequency` and `MaximumFrequency` values of that `PowerSensor`. An acquisition will pause in mid-sweep if the frequency is about to exceed the `MaximumFrequency` value. When the sweep is paused in this manner, a sensor connected to the other channel input of the power meter can be connected to the measurement port in place of the previous sensor, and then the sweep completed by another call to `AcquirePowerReadings`. However, the `MaximumFrequency` specified for the second sensor would need to be sufficient for the sweep to complete.

**Return Type** Boolean

**Default** False (0)

**Examples**

```
Set powerCalibrator = pna.SourcePowerCalibrator
powerCalibrator.UsePowerSensorFrequencyLimits = 1 'Write
FreqCheck = powerCalibrator.UsePowerSensorFrequencyLimits 'Read
```

**C++ Syntax** `HRESULT put_UsePowerSensorFrequencyLimits(VARIANT_BOOL bState);`  
`HRESULT get_UsePowerSensorFrequencyLimits(VARIANT_BOOL *bState);`

**Interface** `ISourcePowerCalibrator`

## UserRange Property

---

**Description** Assigns the marker to the specified User Range. This restricts the marker's x-axis travel to the User Range span, specified with Start and Stop values.

- Each channel has **16** user ranges.
- Markers and trace statistics can be restricted to any user range.
- More than one marker can occupy a user range.
- User ranges can overlap. For example:
  - User range 1 - 3GHz to 5GHz
  - User range 2 - 4GHz to 6GHz

---

**Note:** User ranges are especially useful in restricting marker searches to specific areas of the measurement.

---

**VB Syntax** `mark.UserRange = value`

**Variable** **(Type) - Description**

*mark* A Marker (**object**)

*value* (**long integer**) - User Range. Choose any number between 0 and 16 (0=Full Span)

**Return Type** Long Integer

**Default** 0 - Full Span

**Examples** `mark.UserRange = 1 'Write`

`UserRnge = mark.UserRange 'Read`

**C++ Syntax** HRESULT get\_UserRange(long \*pRangeNumber)  
 HRESULT put\_UserRange(long lRangeNumber)

**Interface** IMarker



## UserRangeMax Property

---

**Description** Sets the stimulus stop value for the specified User Range.  
This property uses different arguments for the channel and marker objects.

**VB Syntax** *chan*.UserRangeMax(*domainType*,*Mnum*) = *value*  
or  
*mark*.UserRangeMax(*rnum*) = *value*

**Variable (Type) - Description**

*chan* A Channel (**object**)

*mark* A Marker (**object**)  
To assign a marker to a User Range, use the [UserRange Property](#).

---

**Note:** The Marker object does not require the "domainType" argument.

---

*domainType* (**enum NADomainType**) - Choose from:

**0** - naDomainFrequency  
**1** - naDomainTime  
**2** - naDomainPower

*Mnum* (**long integer**) - User Range number. Choose any number between 1 and 16 (0=Full Span)

*value* (**double**) - Stop value. Choose any number within the full span of the channel

**Return Type** Double

**Default** The current stimulus setting for the channel

**Examples** `mark.UserRangeMax(1) = 3e9 'Write`  
`chan.UserRangeMax(naDomainFrequency,1) = 3e9 'Write`

```
UseRngeMax = mark.UserRangeMax 'Read
UseRngeMax = chan.UserRangeMax 'Read
```

**C++ Syntax** HRESULT put\_UserRangeMax(tagNADomainType domain, long rangeNumber, double maxValue)  
HRESULT get\_UserRangeMax(tagNADomainType domain, long rangeNumber, double \*maxValue)

**Interface** IChannel

## UserRangeMin Property

---

**Description** Sets the stimulus start value for the specified User Range.

This property uses different arguments for the channel and marker objects.

**VB Syntax** `chan.UserRangeMin(domainType,range) = value`  
**or**  
`mark.UserRangeMin(range) = value`

**Variable** **(Type) - Description**

*chan* A Channel (**object**)

*mark* A Marker (**object**)

To assign a marker to a User Range, use the [UserRange Property](#).

---

**Note:** The Marker object does not require the domainType argument

---

*domainType* **(enum NADomainType)** Type of sweep currently implemented on the channel - Choose from:  
**0 - naDomainFrequency**  
**1 - naDomainTime**  
**2 - naDomainPower**

*range* **(long)** - User Range number. Choose any number between **1** and **16** (0=Full Span)

*value* **(double)** - Start value. Choose any number within the full span of the analyzer

**Return Type** Double

**Default** The current stimulus setting for the channel

**Examples**

```
mark.UserRangeMin(1) = 3e9 'Write
chan.UserRangeMin(naDomainFrequency,1) = 3e9 'Write
```

```
UserRngeMin = mark.UserRangeMin 'Read
UserRngeMin = chan.UserRangeMin 'Read
```

**C++ Syntax** HRESULT put\_UserRangeMin(tagNADomainType domain, long rangeNumber, double minValue)  
 HRESULT get\_UserRangeMin(tagNADomainType domain, long rangeNumber, double \*minValue)

**Interface** IChannel

## UserPresetEnable Property

---

**Description** 'Checks' and 'clears' the enable box on the User Preset dialog box. This only affects subsequent Presets from the front panel user interface.

Regardless of the state of the User Preset Enable checkbox, the `app.Preset` command will always preset the PNA to the factory preset settings, and `app.UserPreset` will always perform a User Preset.

**VB Syntax** `app.UserPresetEnable = state`

**Variable (Type) - Description**

`app` An Application (**object**)

`state` (**boolean**) Front Panel User Preset State. Choose from:

0 (False) – User Preset OFF

1 (True) – User Preset ON

**Return Type** Boolean

**Default** OFF (0)

**Examples** `app.UserPresetEnable = True 'Write`

`upreset = app.UserPresetEnable 'Read`

**C++ Syntax** HRESULT get\_UserPresetEnable(VARIANT\_BOOL \*pVal)  
 HRESULT put\_UserPresetEnable(VARIANT\_BOOL newVal)

**Interface** IApplication6

Read only

## ValidConnectorTypes Property

---

**Description** Returns a list of connector types for which there are calibration kits.

**VB Syntax** *value* = *obj*.ValidConnectorTypes

**Variable** **(Type) - Description**

*value* (Variant) List of connector types

*obj* Any of the following:

[GuidedCalibration](#) (object)

[SMCType](#) (object)

[VMCType](#) (object)

**Return Type** Variant

**Default** Not Applicable

**Examples** `value = SMC.ValidConnectorTypes`

**C++ Syntax** HRESULT get\_ValidConnectorTypes(VARIANT\* connectorTypes);

**Interface** IGuidedCalibration  
SMCType  
VMCType

Write/Read

## VelocityFactor Property

---

**Description** Sets the velocity factor to be used with Electrical Delay, Port Extensions, and Time Domain marker distance calculations.

**VB Syntax** `app.VelocityFactor = value`

**Variable (Type) - Description**

*app* An Application (**object**)

*value* (**double**) - Velocity factor. Choose a number between: **0** and **10**  
(.66 polyethylene dielectric; .7 teflon dielectric)

**Return Type** Double

**Default** 1

**Examples** `app.VelocityFactor = .66 'Write`

`RelVel = app.VelocityFactor 'Read`

**C++ Syntax** HRESULT get\_VelocityFactor(double \*pVal)  
HRESULT put\_VelocityFactor(double newVal)

**Interface** IApplication

Write/Read

**View Property**

---

**Description** Sets (or returns) the type of trace displayed on the screen.**VB Syntax** *meas.View* = *value***Variable** **(Type) - Description***meas* A measurement (**object**)*value* (**enum NAView**) - Type of trace. Choose from:**0** - naData**1** - naDataAndMemory**2** - naMemory**3** - naNoTrace**Note:** The **naData** trace may reflect the result of a [TraceMath](#) operation.**Return Type** NAView**Default** naData**Examples**

```
meas.View = naData 'Write
```

```
trceview = meas.View 'Read
```

**C++ Syntax** HRESULT get\_View(tagNAView\* pView)  
HRESULT put\_View(tagNAView newView)**Interface** IMeasurement

Write/Read

## Visible Property

---

**Description** Makes the Network Analyzer application visible or not visible. In the Not Visible state, the analyzer cycle time for making measurements can be significantly faster because the display does not process data.

**VB Syntax** `app.Visible = state`

**Variable** (Type) - Description

`app` An Application (**object**)

`state` (**boolean**)  
**0** - Network Analyzer application **NOT** visible  
**1** - Network Analyzer application **IS** visible

**Return Type** Boolean  
0 - Not visible  
1 - Visible

**Default** 1

**Examples** `app.Visible = 0 'Write`

`vis = app.Visible 'Read`

**C++ Syntax** HRESULT get\_Visible(VARIANT\_BOOL \* bVisible)  
HRESULT put\_Visible(VARIANT\_BOOL bVisible)

**Interface** IApplication

## WGCutoffFreq Property

---

**Description** Sets or returns the value of the waveguide cut off frequency.

**VB Syntax** *meas.WGCutoffFreq = value*

**Variable** (Type) - Description

*meas* A Measurement **(object)**

*value* **(double)** - Frequency in Hertz.

**Return Type** Double

**Default** Not Applicable

**Examples** `Print meas.WGCutoffFreq 'prints the value of the waveguide cut off frequency`

**C++ Syntax** HRESULT get\_WGCutoffFreq(double \*pVal);  
HRESULT put\_WGCutoffFreq(double newVal);

**Interface** IMeasurement2



Read-only

## WindowNumber Property

---

**Description** Returns the window number. You might use this property to identify a particular window so that you can create a new Measurement in that window.

**VB Syntax** *value* = *win*.**WindowNumber**

**Variable** **(Type) - Description**

*win* A NAWindow (object)

*value* **(long integer)** - Variable to store the returned window number

**Return Type** Long Integer

**Default** Not Applicable

**Examples** `value = app.ActiveNAWindow.WindowNumber`

**C++ Syntax** HRESULT (long\* windowNumber);

**Interface** INAWindow

## WindowState Property

---

**Description** Sets or returns the window setting of Maximized, Minimized, or Normal. To arrange all of the windows, use `app.ArrangeWindows`.

**VB Syntax** `object.WindowState = value`

**Variable** **(Type) - Description**

*object* An Application (object) - main window  
**or**  
 A NaWindow (**object**) - data windows

*value* **(enum NAWindowStates)** - The window state. Choose from:  
**0 - naMinimized** - Minimizes the window to an Icon on the lower toolbar  
**1 - naMaximized** - Maximizes the window  
**2 - naNormal** - changes the window size to the user defined setting (between Max and Min).

**Return Type** Long Integer

**Default** naMaximized

**Examples**

```
app.WindowState = naMinimized 'changes the Network Analyzer application
window to an icon. -Write
win.WindowState = naNormal 'changes the window defined by the win object
variable to user defined settings. -Write
```

```
winstat = app.WindowState 'Read
```

**C++ Syntax** HRESULT get\_WindowState(tagNAWindowStates \*pVal)  
 HRESULT put\_WindowState(tagNAWindowStates newVal)

**Interface** INAWindow  
 IApplication

Write/Read

## XAxisPointSpacing Property

---

**Description** Sets X-axis Point Spacing for the displaytraces measured with segment sweeps on the active channel.

**VB Syntax** `chan.XAxisPointSpacing = value`

**Variable** **(Type) - Description**

*chan* A Channel (**object**)

*value* **(Enum as naStates)** - Choose from:

**0 - naOFF** - Turns X-axis Point Spacing OFF

**1 - naON** - Turns X-axis Point Spacing ON

**Return Type** Enum

**Default** 0 - naOFF

**Examples** `chan.XAxisPointSpacing = naOFF 'Write`

`xspac = chan.XAxisPointSpacing 'Read`

**C++ Syntax** HRESULT get\_XAxisPointSpacing (tagNAStates \*pState);  
HRESULT put\_XAxisPointSpacing (tagNAStates newState);

**Interface** IChannel2

Write/Read

## YScale Property

---

**Description** Sets or returns the Y-axis Per-Division value of the active trace.

**VB Syntax** `trace.YScale = value`

**Variable** (Type) - Description

*trace* A Trace (**object**)

*value* (**double**) - Scale /division number. Units and range depend on the current data format.

**Return Type** Double

**Default** 10 (db)

**Examples** `trac.YScale = 5 'Write`

`yscl = trac.YScale 'Read`

**C++ Syntax** HRESULT get\_YScale(double \*pVal)  
HRESULT put\_YScale(double newVal)

**Interface** ITrace

Write/Read

## Z0 Property

---

**Description** Sets and Returns the characteristic impedance for the calibration standard.

**VB Syntax** `calstd.Z0 = value`

**Variable** (Type) - Description

*calstd* A CalStandard (**object**). Use `calKit.GetCalStandard` to get a handle to the standard.

*value* (**single**) -Impedance in Ohms

**Return Type** Single

**Default** Not Applicable

**Examples** `calstd.Z0 = 50 'Write`

`impedance = calstd.Z0 'Read`

**C++ Syntax** HRESULT get\_Z0(float \*pVal)  
HRESULT put\_Z0(float newVal)

**Interface** ICalStandard

**Description** Ends the current measurement sweep on the channel.

**VB Syntax** `chan.Abort [sync]`

**Variable** **(Type) - Description**

`chan` **(object)** - A Channel object

`sync` **(boolean)** - wait (or not) for the analyzer to stop before processing subsequent commands. Optional argument; if unspecified, value is set to False. Choose from:  
**True** - synchronize - the analyzer will not process subsequent commands until the current measurement is aborted.  
**False** - continue processing commands immediately

**Return Type** None

**Default** None

**Examples** `chan.abort True`  
`chan.abort`

**C++ Syntax** HRESULT Abort(VARIANT\_BOOL bSynchronize);

**Interface** IChannel

**AbortPowerAcquisition Method**

---

**Description** Aborts a source power cal acquisition sweep that is currently in progress.

**VB Syntax** *powerCalibrator*.**AbortPowerAcquisition**

**Variable** (Type) - Description

*powerCalibrator* **(object)** - A SourcePowerCalibrator object

**Return Type** None

**Default** Not Applicable

**Examples** `powerCalibrator.AbortPowerAcquisition`

**C++ Syntax** HRESULT AbortPowerAcquisition();

**Interface** ISourcePowerCalibrator

Write-only

**AcquireCalStandard Method - Obsolete**

---

|                    |                                                                                                                                                                                                                                                                                           |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This command has been replaced by <u>AcquireCalStandard2 Method</u> , which provides for acquisition of sliding load standards. All other functionality is identical.                                                                                                        |
| <b>VB Syntax</b>   | <i>cal.AcquireCalStandard</i> <i>std[,index]</i>                                                                                                                                                                                                                                          |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                               |
| <i>cal</i>         | A Calibrator ( <b>object</b> )                                                                                                                                                                                                                                                            |
| <i>std</i>         | <b>(enum NACalClass)</b> Standard to be measured. Choose from: <ul style="list-style-type: none"> <li>1 - naClassA</li> <li>2 - naClassB</li> <li>3 - naClassC</li> <li>4 - naClassD</li> <li>5 - naClassE</li> <li>6 - naReferenceRatioLine</li> <li>7 - naReferenceRatioThru</li> </ul> |
|                    | <b>SOLT Standards</b> <ul style="list-style-type: none"> <li>1 - naSOLT_Open</li> <li>2 - naSOLT_Short</li> <li>3 - naSOLT_Load</li> <li>4 - naSOLT_Thru</li> <li>5 - naSOLT_Isolation</li> </ul>                                                                                         |
|                    | <b>TRL Standards</b> <ul style="list-style-type: none"> <li>1 - naTRL_Reflection</li> <li>2 - naTRL_Line_Reflection</li> <li>3 - naTRL_Line_Tracking</li> <li>4 - naTRL_Thru</li> <li>5 - naTRL_Isolation</li> </ul>                                                                      |
| <i>index</i>       | <b>(long integer)</b> number of the standard. Optional argument - Used if there is more than one standard required to cover the necessary frequency range. If unspecified, value is set to 1.                                                                                             |
| <b>Return Type</b> | None                                                                                                                                                                                                                                                                                      |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                            |



---

**Examples** `Cal.AcquireCalStandard naSOLT_Thru 'Write`

---

**C++ Syntax** HRESULT AcquireCalStandard(tagNACalClass enumClass, short standardNumber)

**Interface** ICalibrator

## AcquireCalStandard2 Method

---

**Description** Measures the specified standard from the selected calibration kit. The calibration kit is selected using [app.CalKitType](#).

For 2-port calibration, it is also necessary to specify direction with [AcquisitionDirection](#).

To omit Isolation from a 2-port calibration, do not Acquire a cal standard for naSOLT\_Isolation.

For using two sets of standards, see [Simultaneous2PortAcquisition Property](#).

**Note:** This command replaces [AcquireCalStandard](#). This command provides for the acquisition of a sliding load cal. All other functionality is identical.

---

**VB Syntax** *cal.AcquireCalStandard2 std[,index][,slide]*

**Variable (Type) - Description**

*cal* A [Calibrator](#) (**object**)

*std* (**enum NACalClass**) Standard to be measured. Choose from:

1 - naClassA

2 - naClassB

3 - naClassC

4 - naClassD

5 - naClassE

6 - naReferenceRatioLine

7 - naReferenceRatioThru

### SOLT Standards

1 - naSOLT\_Open

2 - naSOLT\_Short

3 - naSOLT\_Load

4 - naSOLT\_Thru

5 - naSOLT\_Isolation

### TRL Standards

1 - naTRL\_Reflection

2 - naTRL\_Line\_Reflection

3 - naTRL\_Line\_Tracking

4 - naTRL\_Thru

5 - naTRL\_Isolation

*[index]* **(long integer)** Number of the standard. Optional argument - Used if there is more than one standard required to cover the necessary frequency range. If unspecified, value is set to 1.

*[slide]* **(enum as NACalStandardSlidingState)** Optional argument. State of the sliding load. The slide should be set a minimum of five times. Seven is the maximum that can be stored. Choose from:

0 - **naNotSlidingStd** - not using a sliding load - Default if not specified.

1 - **naSlidelsSet** - slide is set for acquisition

2 - **naSlidelsDone** - this next acquisition will be the last. Calculations will then be performed.

**Return Type** None

**Default** Not Applicable

**Examples** `Cal.AcquireCalStandard2 naSOLT_Thru`  
`Cal.AcquireCalStandard2 naSOLT_Thru,2,naNotSlidingStd`  
`'measures the second standard listed in the class of naSOLT_Thru`

**C++ Syntax** HRESULT AcquireCalStandard2(NACalClass enumClass, long standardPosition, NACalStandardSlidingState slidingStandardState)

**Interface** ICalibrator

## AcquireCalConfidenceCheckECALEX Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p>This method replaces <a href="#">AcquireCalConfidenceCheckECAL</a></p> <p>Transfers confidence data from the specified ECal module into the measurement's memory trace. The data is transferred to the specified S-parameter on the same channel as this Calibrator object.</p> <p>The characterization within the ECal module that the confidence data will be read from is specified by <a href="#">ECALCharacterizationEx</a>. The default value is 0.</p> |
| <b>VB Syntax</b>   | <i>cal.AcquireCalConfidenceCheckECALEX</i> <i>Sparam</i> [, <i>ecalModule</i> ]                                                                                                                                                                                                                                                                                                                                                                                  |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <i>cal</i>         | A Calibrator <b>(object)</b>                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <i>Sparam</i>      | <b>(String)</b> S-parameter to transfer confidence data to. This parameter must be present on the same channel as the calibrator object.                                                                                                                                                                                                                                                                                                                         |
| <i>ecalModule</i>  | <p><b>(Integer)</b> – Optional argument. ECal module.</p> <p>Choose from modules <b>1</b> through <b>8</b></p> <p>Use <a href="#">IsECALModuleFoundEx</a> to determine the number of modules connected to the PNA</p> <p>Use <a href="#">GetECALModuleInfoEx</a> to return the model and serial number of each module.</p>                                                                                                                                       |
| <b>Return Type</b> | None                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| <b>Default</b>     | Not applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                   |
| <b>Examples</b>    | <code>Cal.AcquireCalConfidenceCheckECALEX "S11", 2</code>                                                                                                                                                                                                                                                                                                                                                                                                        |
| <b>C++ Syntax</b>  | HRESULT AcquireCalConfidenceCheckECALEX(BSTR strParameter, long moduleNumber = 1);                                                                                                                                                                                                                                                                                                                                                                               |
| <b>Interface</b>   | ICalibrator4                                                                                                                                                                                                                                                                                                                                                                                                                                                     |

## AcquirePowerReadings Method

---

**Description** Initiates a source power cal acquisition.

**VB Syntax** `powerCalibrator.AcquirePowerReadings device [,sync]`

**Variable** **(Type) - Description**

*powerCalibrator* **(object)** - A SourcePowerCalibrator object

*device* **(enum NAPowerAcquisitionDevice)** The specific device (sensor on the power meter) to be used for the acquisition. Choose from:

**0 – naPowerSensor\_A**

**1 – naPowerSensor\_B**

To use the sensor that currently corresponds to the frequency of interest, use the value from the PowerAcquisitionDevice property.

*sync* **(boolean)** Optional argument. If not specified, value is set to False. Choose from:

**True (1)** – The method does not return until this acquisition has completed (the program calling this method is halted while waiting for the method to return).

**False (0)** – The method initiates an acquisition then returns immediately (while the acquisition still proceeds). The program calling this method can then perform other operations during the acquisition.

**Return Type** None

**Default** Not Applicable

**Examples** `powerCalibrator.AcquirePowerReadings naPowerSensor_A, True`

**C++ Syntax** `HRESULT AcquirePowerReadings(tagNAPowerAcquisitionDevice enumAcqDevice, VARIANT_BOOL bSync);`

**Interface** ISourcePowerCalibrator

Write-only

## AcquireStep Method

---

**Description** Acquire the measurement data for the specified step in the calibration process.

**VB Syntax** `obj.AcquireStep (n)`

**Variable** **(Type) - Description**

*obj* Any of the following:  
[GuidedCalibration](#) (object)  
[SMCType](#) (object)  
[VMCType](#) (object)

*n* Step number in the calibration process.  
Use [GenerateSteps](#) to determine the total number of steps.  
Use [GetStepDescription](#) to read the description of each step.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `VMC.AcquireStep (3)`

**C++ Syntax** `HRESULT put_AcquireStep([in] long step);`

**Interface** SMCType  
VMCType  
IGuidedCalibration

## Activate Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Makes an object the Active Object. When making a measurement active, the channel and window the measurement is contained in becomes the active channel and active window.<br><br>In order to change properties on any of the active objects, you must first have a "handle" to the active object using the <b>Set</b> command. For more information, See <a href="#">Getting a Handle to an Object</a> .<br><br>You do not have to make an object "Active" to set or read its properties remotely. But an object must be "Active" to change its values from the front panel. |
| <b>VB Syntax</b>   | <i>object</i> . <b>Activate</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <i>object</i>      | <u>Measurement</u> <b>(object)</b><br><b>or</b><br><u>Marker</u> <b>(object)</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <b>Examples</b>    | <code>meas.Activate</code><br><code>mark.Activate</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>C++ Syntax</b>  | HRESULT Activate()                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Interface</b>   | IMeasurement<br>IMarker                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |

## ActivateMarker Method

---

|                    |                                                                                                                       |
|--------------------|-----------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Makes a marker the Active Marker. Use <code>meas.ActiveMarker</code> to read the number of the active marker.         |
| <b>VB Syntax</b>   | <code>meas.ActiveMarker(Mnum)</code>                                                                                  |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                           |
| <i>meas</i>        | A <u>Measurement</u> ( <b>object</b> )                                                                                |
| <i>Mnum</i>        | <b>(long integer)</b> - the number of the marker to make active. Choose any marker number from <b>1</b> to <b>9</b> . |
| <b>Return Type</b> | None                                                                                                                  |
| <b>Default</b>     | Not Applicable                                                                                                        |
| <b>Examples</b>    | <code>meas.ActiveMarker(1) 'Write</code>                                                                              |
| <b>C++ Syntax</b>  | <code>HRESULT ActivateMarker(long IMarkerNumber)</code>                                                               |
| <b>Interface</b>   | IMeasurement                                                                                                          |
| <b>Remarks</b>     | Use <u>ReferenceMarkerState</u> to control the Reference marker.                                                      |



## ActivateWindow Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|--------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Makes a window object the Active Window.<br><br>In order to change properties on any of the active objects, you must first have a "handle" to the active object using the <b>Set</b> command. For more information, See <a href="#">Programming the Analyzer Object Model</a> .<br><br>You do not have to make an object "Active" to set or read its properties remotely. But an object must be "Active" to change its values from the front panel. |
| <b>VB Syntax</b>   | <code>app.ActivateWindow n</code>                                                                                                                                                                                                                                                                                                                                                                                                                   |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                         |
|                    | <code>app</code> An <a href="#">Application</a> ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                                                                   |
|                    | <code>n</code> ( <b>long</b> ) Number of the window to make active                                                                                                                                                                                                                                                                                                                                                                                  |
| <b>Return Type</b> | Window Object                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>Examples</b>    | <code>app.ActivateWindow 4</code>                                                                                                                                                                                                                                                                                                                                                                                                                   |
| <b>C++ Syntax</b>  | <code>HRESULT ActivateWindow(long WindowNumber)</code>                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Interface</b>   | IApplication                                                                                                                                                                                                                                                                                                                                                                                                                                        |

## Add (channels) Method

---

|                    |                                                                                                                             |
|--------------------|-----------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Creates a channel and returns a handle to it. If the channel already exists, it returns the handle to the existing channel. |
| <b>VB Syntax</b>   | <i>chans.Add (item)</i>                                                                                                     |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                 |
| <i>chans</i>       | A <u>Channel collection</u> <b>(object)</b>                                                                                 |
| <i>item</i>        | <b>(variant)</b> - Channel number.                                                                                          |
| <b>Return Type</b> | Channel                                                                                                                     |
| <b>Default</b>     | Not Applicable                                                                                                              |
| <b>Examples</b>    | <code>chans.Add 3 'Creates channel 3</code>                                                                                 |
| <b>C++ Syntax</b>  | HRESULT Add(VARIANT numVal, IChannel** pChannel)                                                                            |
| <b>Interface</b>   | IChannels                                                                                                                   |

## Write-only

### Add (measurement) Method

---

**Description** Adds a Measurement to the collection.

**VB Syntax** `meas.Add channel,param,source[,window]`

*meas* A Measurements collection (**object**)

*channel* (**long**) - Channel number of the new measurement.

*param* (**string**) - Parameter of the new measurement. Choose from:

- "S11"
- "S22"
- "S21"
- "S12"
- "A"
- "B"
- "R1"
- "R2"

or

- combine 2 of (A,B,R1,R2) in this format: "A/R1"

*source* (**long integer**) - Source port number; if unspecified, value is set to 1. Only used for non-s-parameter measurements; ignored if s-parameter.

*window* (**long integer**) - Optional argument. Window number of the new measurement. Choose 1 to 16. If unspecified, the S-Parameter will be created in the Active Window.

**Return Type** None

**Default** None

**Examples** `meass.Add 3,"A/R1",1,1 'Adds A/R1 measurement to channel 3 in window 1`

**C++ Syntax** `HRESULT Add(long ChannelNum, BSTR strParameter, long srcPort, VARIANT_BOOL bNewWindow)`

**Interface** IMeasurements

## Add (NAWindows) Method

---

|                    |                                                                                                    |
|--------------------|----------------------------------------------------------------------------------------------------|
| <b>Description</b> | Add a window to the display. Does not add a measurement. The window number must not already exist. |
| <b>VB Syntax</b>   | <code>wins.Add [item]</code>                                                                       |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                        |
| <code>wins</code>  | A <a href="#">NAWindow</a> collection ( <b>object</b> )                                            |
| <code>item</code>  | <b>(variant)</b> - optional argument; Window number. Range between 1 - 16                          |
| <b>Return Type</b> | Object                                                                                             |
| <b>Default</b>     | Not Applicable                                                                                     |
| <b>Examples</b>    | <code>wins.Add 3 'Creates a window number 3</code>                                                 |
| <b>C++ Syntax</b>  | <code>HRESULT Add(long windowNumber )</code>                                                       |
| <b>Interface</b>   | INAWindows                                                                                         |

## Add (PowerLossSegment) Method

---

- Description** Adds a PowerLossSegment to the PowerLossSegments collection.  
To ensure predictable results, it is best to remove all segments before defining a new list of segments. For each segment in the collection, do a [seg.Remove](#).
- VB Syntax** `segs.Add (item [ size])`
- Variable** **(Type) - Description**
- `segs` **(object)** - A [PowerLossSegments](#) collection (object)
- `item` **(variant)** - Number of the new segment. If it already exists, a new segment is inserted at the requested position.
- `size` **(long integer)** - Optional argument. The number of segments to add, starting with item. If unspecified, value is set to 1.
- Return Type** None
- Default** Not Applicable
- Examples** `segs.Add 1, 4 'Adds segments 1,2,3 and 4`
- C++ Syntax** HRESULT Add(VARIANT index, long size);
- Interface** IPowerLossSegments

## Add (PowerSensorCalFactorSegment) Method

---

- Description** Adds a PowerSensorCalFactorSegment to the CalFactorSegments collection.  
To ensure predictable results, it is best to remove all segments before defining a new list of segments. For each segment in the collection, do a [seg.Remove](#).
- VB Syntax** `segs.Add (item [ size])`
- Variable** **(Type) - Description**
- `segs` **(object)** - A [CalFactorSegments](#) collection (object)
- `item` **(variant)** - Number of the new segment. If it already exists, a new segment is inserted at the requested position.
- `size` **(long integer)** - Optional argument. The number of segments to add, starting with item. If unspecified, value is set to 1.
- Return Type** None
- Default** Not Applicable
- Examples** `segs.Add 1, 4 'Adds segments 1,2,3 and 4`
- C++ Syntax** HRESULT Add(VARIANT index, long size);
- Interface** ICalFactorSegments

Write-only

**Add (segment) Method**

---

**Description** Adds segments to the Segments collection, but does not turn the segments ON.**VB Syntax** `segs.Add (item, [size])`*segs* A segments collection (**object**)*item* (**variant**) Number of the new segment. If it already exists, a new segment is inserted at the requested position.*size* (**long integer**) Optional argument. The number of segments to add, starting with *item*. If unspecified, value is set to 1.**Return Type** None**Default** None**Examples** `Segs.Add 1, 4 'Adds segments 1,2,3,and 4. (does NOT automatically turn segments ON)`**C++ Syntax** HRESULT Add(VARIANT index, long size);**Interface** ISegments**Remarks** To ensure predictable results, it is best to remove all segments before defining a segment list. For each segment in the collection, do a `seg.Remove`.

**AllowAllEvents Method**

---

|                    |                                                                                                                                                                                          |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Sets event filtering to monitor all events in the analyzer. This is the default setting when subscribing to events. This could slow the measurement speed of the analyzer significantly. |
| <b>VB Syntax</b>   | <i>app</i> .AllowAllEvents                                                                                                                                                               |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                              |
|                    | <i>app</i> An <u>Application</u> ( <b>object</b> )                                                                                                                                       |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                           |
| <b>Default</b>     | Not Applicable                                                                                                                                                                           |
| <b>Examples</b>    | <code>app.AllowAllEvents</code>                                                                                                                                                          |
| <b>C++ Syntax</b>  | HRESULT AllowAllEvents()                                                                                                                                                                 |
| <b>Interface</b>   | IApplication                                                                                                                                                                             |



## AllowEventCategory Method

---

**Description** Sets event filtering to monitor a category of event.

**VB Syntax** `app.AllowEventCategory, category, state`

**Variable** **(Type) - Description**

*app* An Application (**object**)

*category* Category to monitor. Choose from list in Working with the Analyzer's Events

*state* **(boolean)**  
**True** - monitor  
**False** - do not monitor

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.AllowEventCategory`

**C++ Syntax** HRESULT AllowEventCategory(tagNAEventCategory category, VARIANT\_BOOL bAllow )

**Interface** IApplication

**AllowEventMessage Method**

---

|                    |                                                                              |
|--------------------|------------------------------------------------------------------------------|
| <b>Description</b> | Sets event filtering to monitor specific events.                             |
| <b>VB Syntax</b>   | <i>app.AllowEventMessage event</i>                                           |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                  |
| <i>app</i>         | An <u>Application</u> ( <b>object</b> )                                      |
| <i>event</i>       | Event to monitor. Refer to list in <u>Working with the Analyzer's Events</u> |
| <i>state</i>       | <b>(boolean)</b><br><b>True</b> - monitor<br><b>False</b> - do not monitor   |
| <b>Return Type</b> | Not Applicable                                                               |
| <b>Default</b>     | Not Applicable                                                               |
| <b>Examples</b>    | <code>app.AllowEventMessage</code>                                           |
| <b>C++ Syntax</b>  | HRESULT AllowEventMessage( tagNAEventID eventID, VARIANT_BOOL bAllow)        |
| <b>Interface</b>   | IApplication                                                                 |

**AllowEventSeverity Method**

---

|                    |                                                                                                                                                    |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Sets event filtering to monitor levels of severity.                                                                                                |
| <b>VB Syntax</b>   | <i>app.AllowEventSeverity severity,state</i>                                                                                                       |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                        |
| <i>app</i>         | An <u>Application</u> ( <b>object</b> )                                                                                                            |
| <i>severity</i>    | <b>(enum naEventSeverity)</b> Choose from:naEventSeverityERROR<br>naEventSeverityINFORMATIONAL<br>naEventSeveritySUCCESS<br>naEventSeverityWARNING |
| <i>state</i>       | <b>(boolean)</b><br><b>True</b> - monitor<br><b>False</b> - do not monitor                                                                         |
| <b>Return Type</b> | Not Applicable                                                                                                                                     |
| <b>Default</b>     | Not Applicable                                                                                                                                     |
| <b>Examples</b>    | <code>app.AllowEventSeverity</code>                                                                                                                |
| <b>C++ Syntax</b>  | HRESULT AllowEventSeverity( tagNAEventSeverity severity, VARIANT_BOOL bAllow)                                                                      |
| <b>Interface</b>   | IApplication                                                                                                                                       |

Write only

## Apply Method

---

**Description** Applies the mixer setup to the mixer object and turns the channel ON. (Performs the same function as the Apply button on the mixer setup dialog box.)

**VB Syntax** *mxr*.Apply

**Variable** (Type) - Description

*mxr* Mixer Interface pointer to the Measurement (object)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mxr.Apply`

**C++ Syntax** HRESULT Apply()

**Interface** IMixer3

## ApplyPowerCorrectionValues Method

---

**Description** Applies the array of power correction values to the channel memory and turns correction ON. Perform after completing a source power cal acquisition sweep.

This command does NOT save the correction values. To save correction values, save an instrument / calibration state (\*.cst file) after performing a source power cal.

**VB Syntax** `powerCalibrator.ApplyPowerCorrectionValues`

**Variable** **(Type) - Description**

`powerCalibrator` **(object)** - A SourcePowerCalibrator object

**Return Type** None

**Default** Not Applicable

**Examples** `powerCalibrator.ApplyPowerCorrectionValues`

**C++ Syntax** `HRESULT ApplyPowerCorrectionValues();`

**Interface** `ISourcePowerCalibrator`

## AutoPortExtMeasure Method

---

**Description** Measures either an OPEN or SHORT standard. When this command is sent, the PNA acquires the measurement with which to set automatic port extensions. [Learn more about choosing which standard to measure.](#)

**VB Syntax** *fixture*.AutoPortExtMeasure *value*

**Variable** **(Type) - Description**

*fixture* A [Fixturing](#) (**object**)

*value* (Enum as NAAutoPortExtMeasure)

0 - naAPEM\_OPEN - Measure OPEN

1 - naAPEM\_SHORT - Measure SHORT

**Return Type** ENUM

**Default** Not Applicable

**Examples** `fixture.AutoPortExtMeasure naAPEM_OPEN`

**C++ Syntax** HRESULT get\_AutoPortExtMeasure(tagNAAutoPortExtMeasure \*pVal );

**Interface** IFixturing2

## AutoPortExtReset Method

---

|                    |                                                                                                                                                                                                                                                                                                |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Clears old port extension delay and loss data in preparation for acquiring new data. Send this command prior to sending a new series of measurements using <u>AutoPortExtMeasure Method</u> . If acquiring both OPEN and SHORT standards, do not send this command between those acquisitions. |
| <b>VB Syntax</b>   | <i>fixture</i> .AutoPortExtReset                                                                                                                                                                                                                                                               |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                    |
| <i>fixture</i>     | A <u>Fixturing</u> ( <b>object</b> )                                                                                                                                                                                                                                                           |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                 |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                 |
| <b>Examples</b>    | <code>fixture.AutoPortExtReset</code>                                                                                                                                                                                                                                                          |
| <b>C++ Syntax</b>  | HRESULT AutoPortExtReset();                                                                                                                                                                                                                                                                    |
| <b>Interface</b>   | IFixturing2                                                                                                                                                                                                                                                                                    |

## Autoscale Method

---

|                    |                                                                                                                                                                                                    |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Trace Object - Autoscales only the <b>ONE</b> trace on which Autoscale is being called.<br>NAWindow Object - Autoscales <b>ALL</b> of the traces in the Window on which Autoscale is being called. |
| <b>VB Syntax</b>   | <i>object</i> . <b>Autoscale</b>                                                                                                                                                                   |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                        |
|                    | <i>object</i> <u>Trace</u> <b>(object)</b><br><b>or</b><br><u>NAWindow</u> <b>(object)</b>                                                                                                         |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                     |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                     |
| <b>Examples</b>    | <pre>Trac.Autoscale 'Autoscales the trace<br/>Win.Autoscale 'Autoscales all the traces in the window -Write</pre>                                                                                  |
| <b>C++ Syntax</b>  | HRESULT AutoScale()                                                                                                                                                                                |
| <b>Interface</b>   | INAWindow<br>ITrace                                                                                                                                                                                |



## AveragingRestart Method

---

**Description** Clears and restarts averaging of the measurement data.

**VB Syntax** `chan.AveragingRestart`

**Variable** **(Type) - Description**

`chan` A Channel (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `chan.AveragingRestart`

**C++ Syntax** HRESULT AveragingRestart()

**Interface** IChannel

Write-only

**BuildHybridKit Method**

---

|                                    |                                                                                                                                                                                                                                                                                                                          |
|------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b>                 | Use this method when you have different port connectors. This is a convenient way to combine two kits that match the connectors on your DUT.                                                                                                                                                                             |
| <b>VB Syntax</b>                   | <i>app</i> .BuildHybridKit <i>port1Kit,p1sex,port2Kit,p2sex,adapter,user kit</i>                                                                                                                                                                                                                                         |
| <b>Variable</b>                    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                              |
| <i>app</i>                         | An <u>Application</u> ( <b>object</b> )                                                                                                                                                                                                                                                                                  |
| <i>port1Kit</i><br><i>port2Kit</i> | <b>(enum NACalKit)</b> - Specifies the two kits to be used to build the hybrid kit. Choose from:<br>naCalKit_85032F_N50<br>naCalKit_85033E_3_5<br>naCalKit_85032B_N50<br>naCalKit_85033D_3_5<br>naCalKit_85038A_7_16<br>naCalKit_85052C_3_5_TRL<br>naCalKit_User7<br>naCalKit_User8<br>naCalKit_User9<br>naCalKit_User10 |
| <i>p1sex</i><br><i>p2sex</i>       | <b>(enum NAPortSex)</b> - Specifies the sex of the connector at that port. Choose from:<br>naMale<br>naFemale<br>naDon'tCare                                                                                                                                                                                             |
| <i>adapter</i>                     | <b>(enum NAAadapter)</b> -Choose from:<br>naUserkit - the electrical length of the adapter in the userKit specifications<br>naZeroLength - no adapter                                                                                                                                                                    |
| <i>userKit</i>                     | <b>(enum NACalKit)</b> - The Hybrid kit - Choose from the previous list of kits                                                                                                                                                                                                                                          |
| <b>Return Type</b>                 | Not Applicable                                                                                                                                                                                                                                                                                                           |
| <b>Default</b>                     | Not Applicable                                                                                                                                                                                                                                                                                                           |
| <b>Examples</b>                    | <pre>app.BuildHybridKit naCalKit_85033E_3_5,naMale,naCalKit_85038A_7_16 ,naFemale,naUserkit,naCalKit_User8</pre>                                                                                                                                                                                                         |
| <b>C++ Syntax</b>                  | HRESULT BuildHybridKit(tagNACalKit port1Kit, tagNAPortSex port1Sex, tagNACalKit port2Kit, tagNAPortSex port2Sex, tagNAAadapter adapter, tagNACalKit userKit)                                                                                                                                                             |
| <b>Interface</b>                   | IApplication                                                                                                                                                                                                                                                                                                             |

Write-only

## CalculateErrorCoefficients Method

---

**Description** This method is the final call in a calibration process. It calculates error-correction terms and turns error-correction ON.

Do NOT use this command during an ECAL.

**VB Syntax** *cal*.**CalculateErrorCoefficients**

**Variable** (Type) - Description

*cal* Calibrator (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `Cal.CalculateErrorCoefficients`

**C++ Syntax** HRESULT CalculateErrorCoefficients()

**Interface** ICalibrator

## Calculate Method

---

**Description** Calculates the Input or Output frequencies of the mixer setup, applies the mixer setup to the mixer object, and turns the channel ON.

**VB Syntax** *mxr.Calculate* (*port*)

**Variable** **(Type) - Description**

*mxr* Mixer Interface pointer to the Measurement (object)

*port* (enum as MixerCalculation) Port of the mixer for which to calculate start and stop frequencies. Choose from:

|   | enum                                                 | 1st or only stage requires:                                                                                                                               | In addition, 2nd stage requires:                                                                                                                   |
|---|------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------|
| 0 | mixCalculateINPUT                                    | <ul style="list-style-type: none"> <li>• Output Start and Stop frequencies</li> <li>• LO frequency</li> <li>• Output sideband (High or Low)</li> </ul>    | <ul style="list-style-type: none"> <li>• IF Start and Stop frequencies</li> <li>• 2nd LO frequency</li> <li>• IF sideband (High or Low)</li> </ul> |
| 1 | mixCalculateINPUT AndOUTPUT<br>(2 stage mixers ONLY) | NA                                                                                                                                                        | <ul style="list-style-type: none"> <li>• IF Start and Stop frequencies</li> <li>• Both LO frequencies</li> </ul>                                   |
| 2 | mixCalculateOUTPUT                                   | <ul style="list-style-type: none"> <li>• Input Start and Stop frequencies</li> <li>• LO frequency</li> <li>• Output sideband (High or Low)</li> </ul>     | <ul style="list-style-type: none"> <li>• IF Start and Stop frequencies</li> <li>• 2nd LO frequency</li> <li>• IF sideband (High or Low)</li> </ul> |
| 3 | mixCalculateLO1                                      | <ul style="list-style-type: none"> <li>• Input Start and Stop frequencies</li> <li>• Output frequency</li> <li>• Output sideband (High or Low)</li> </ul> | <ul style="list-style-type: none"> <li>• IF Start and Stop frequencies</li> <li>• 2nd LO frequency</li> <li>• IF sideband (High or Low)</li> </ul> |

|   |                 |    |                                                                                                                                                                                                                                           |
|---|-----------------|----|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 4 | mixCalculateLO2 | NA | <ul style="list-style-type: none"> <li>• Input Start and stop frequencies</li> <li>• 1st LO start and stop frequencies</li> <li>• Output frequency</li> <li>• IF sideband(High or Low)</li> <li>• Output sideband(High or Low)</li> </ul> |
|---|-----------------|----|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mxr.Calculate (mixCalculateOUTPUT)`

**C++ Syntax** HRESULT Calculate()

**Interface** IMixer

## ChangeParameter Method

---

**Description** Changes the parameter of the measurement.

**VB Syntax** `meas.ChangeParameter(param,IPort)`

**Variable** **(Type) - Description**

*meas* A Measurement (**object**)

*param* (**string**) - New parameter. Choose from:

**S11 | S22 | S21 | S12**

Additionally, for 3-port analyzers only:

**S33 | S13 | S31 | S23 | S32**

For non-ratioed measurements:

**A | B | R1 | R2**

**C** - 3-port analyzers only

For ratioed measurements:

**A/B**

**A/C** - 3 port analyzers only

**B/A**

**B/C** - 3 port analyzers only

**C/A** - 3 port analyzers only

**C/B** - 3 port analyzers only

**A/R1**

**B/R1**

**C/R1** - 3 port analyzers only

**A/R2**

**B/R2**

**R1/A**

**R2/A**

**R1/B**

**R2/B**

**R1/C** - 3 port analyzers only

**R2/R1**

**R1/R2**

*IPort* **(long integer)**

Load port if *param* is a reflection S-Parameter

Ignored if *param* is a transmission S-Parameter

Source port if *param* is anything other than an S-parameter

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `meas.ChangeParameter "S11",1`

**C++ Syntax** HRESULT ChangeParameter(BSTR parameter, long IPort)

**Interface** IMeasurement

**CheckPower Method**

---

- Description** Measures power at a specified frequency. Use this method to test power level before and/or after applying a source power calibration.
- VB Syntax** `pow = pwrCal.CheckPower (device, freq [,unit])`
- Variable (Type) - Description**
- `pow` **(double)** Variable to store power value returned by this method.
- `pwrCal` A [SourcePowerCalibrator](#) **(object)**
- `device` **(enum NAPowerAcquisitionDevice)** The specific sensor on the power meter to be used for the acquisition. Choose from:
- 0** – naPowerSensor\_A
- 1** – naPowerSensor\_B
- To use the sensor that currently corresponds to the frequency of interest, use the value from the [PowerAcquisitionDevice](#) property.
- `freq` **(double)** Frequency (Hz) at which the sensor is to read the power.
- `unit` **(enum NAPowerUnit)**
- Optional argument. Choose from:
- naDBM** – Returns the power in dBm.(default)
- naWATT** – Returns the power in Watts.
- Return Type** Double
- Default** Not Applicable
- Examples** `watt = powerCalibrator.CheckPower(naPowerSensor_A, 1E9, naWATT)`
- C++ Syntax** `HRESULT put_CheckPower(tagNAPowerAcquisitionDevice enumAcqDevice, double dFreq, tagNAPowerUnit enumPowerUnit, double *pdPower);`
- Interface** ISourcePowerCalibrator2



**CloseCalSet Method OBSOLETE**

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p>This command is no longer necessary. The CalSet.get... and put... commands that required this command have been replaced,</p> <hr/> <p>Closes read/write access to the Cal Set.</p> <p>See <a href="#">OpenCalSet</a> for an explanation of gaining access to the Cal Set.</p> <p>When you are finished reading and writing data from or to the Cal Set, close the Cal Set. Subsequent read/writes will require a new OpenCal Set call.</p> <p>Reading and writing Cal Set data is performed with the PutStandard, GetStandard, PutErrorTerm, GetErrorTerm method calls. These methods are provided by the <a href="#">ICal Set</a> and ICalData2 interfaces.</p> |
| <b>VB Syntax</b>   | <i>CalSet</i> .CloseCalSet                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
|                    | <i>CalSet</i> <b>(object)</b> - A <a href="#">Cal Set</a> object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Examples</b>    | <code>CSet.CloseCalSet</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| <b>C++ Syntax</b>  | HRESULT CloseCalSet                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <b>Interface</b>   | ICalSet                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |

**ComputeErrorTerms Method**

---

**Description** Computes error terms for the caltype specified by a preceding OpenCal Set call.

The Cal Set must first be opened using OpenCalSet. If this call has not been made, the following error is issued:

E\_NA\_Cal Set\_ACCESS\_DENIED

The standards data required for the CalType must be available in the Cal Set or this error will be returned: E\_NA\_STANDARD\_NOT\_FOUND.

---

**Note:** Error term computation requires data for the actual calibration kit standards from the current kit definition. ComputeErrorTerms assumes that the standards were acquired using only one standard per class.

---

**VB Syntax** *CalSet*.**ComputeErrorTerms**

**Variable** (Type) - Description

*CalSet* **(object)** - A Cal Set object

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `CalSet.ComputeErrorTerms`

**C++ Syntax** HRESULT ComputeErrorTerms( )

**Interface** ICalSet

**ConfigNarrowBand2 Method Obsolete**


---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p><b>Note:</b> This method has been replaced by <a href="#">ConfigNarrowBand3 Method</a></p> <hr/> <p>This command replaced <a href="#">ConfigNarrowBand Method</a>. Two additional arguments have been added: FixedPRF and 85110 gen.</p> <hr/> <p>This subroutine determines, then returns, the proper configuration for pulsed measurements on the PNA using the spectral nulling technique. The configuration returned needs to be sent to the PNA and any other related external equipment such as pulse generators. The routine will take a desired Pulse Repetition Frequency (PRF) and measurement IFBW and return a possibly modified PRF and IFBW for proper pulsed operation on the PNA. The routine will also return the Sample Rate, Number of Taps, and Offset that must be sent to the PNA to configure it in pulsed mode using the spectral nulling technique.</p> <p>Although the example below uses COM programming to communicate with the PNA, these commands can be replaced with <a href="#">SCPI equivalents</a>.</p> <hr/> <p><b>Note:</b> The pulsed application may set the offset frequency (option 080) of the PNA to some value other than zero (the default value). If the stop frequency is set to the maximum of the PNA model, then an error message may appear on the PNA stating that the response frequency has exceeded the maximum allowed frequency. To fix this, set the stop frequency to a value that is at least 2 KHz less than the maximum allowed. For example, if you have a 20 GHz PNA, and the stop frequency is set to 20 GHz, and the error message appears, then set the stop frequency to 19.999998 GHz</p> <hr/> |
| <b>VB Syntax</b>   | <i>Pulsed.ConfigNarrowBand</i> ( <i>PRF, NumTaps, BW, OffSet, SampleRate, Precision, FixedPRF, PG81110</i> )                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| <i>Pulsed</i>      | <b>(interface)</b> An interface to the agilentpnapulsed.dll application interface.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <i>PRF</i>         | <b>(Double)</b> The Pulse Repetition Frequency.<br><b>[out]</b> The pulse repetition frequency that has been optimized for use with the PNA. NOTE: This value may be different from the value requested.<br><b>[in]</b> The desired pulse repetition frequency.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <i>NumTaps</i>     | <b>(Long)</b> The number of taps to send to the PNA for pulsed operation.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <i>BW</i>          | <b>(Long)</b> The PNA IF Bandwidth.<br><b>[out]</b> The PNA IF bandwidth that has been optimized for use with the PNA. NOTE: This value may be different from the value requested.<br><b>[in]</b> The desired PNA IF bandwidth.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <i>Offset</i>      | <b>(Double)</b> The offset value to send to the PNA for pulsed operation. The offset value is used to adjust the PNA for the two different possible sample rates that may be returned.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <i>SampleRate</i>  | <b>(Double)</b> The sample rate to send to the PNA for pulsed operation.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |

*Precision* **(Double)** The precision variables sets the precision that will be used to decrement the PRF when running the configuration routines. This variable can be set to the precision required by the external pulse generators so that the configuration routine will not return a PRF that is not within the precision limits of the pulse generators.

*FixedPRF* **(Boolean)**

**1 (True)** Signals the .DLL routine to NOT adjust the PRF value; rather adjust ONLY the IF Bandwidth. This is the default setting.

**0 (False)** Adjust both the PRF and IF Bandwidth values as necessary.

*PG81110* **(Boolean)**

**1 (True)** You are using an Agilent 81110 as the pulse generator. This allows increased accuracy in adjustments for offset and PRF.

**0 (False)** Not using an Agilent 81110.

**Return Type** Not Applicable

**Default** Not Applicable

**Example** [See an example using this command.](#)

**C++ Syntax** HRESULT ConfigNarrowBand(double \*pPRF, long \*pNumTaps, long \*pBW, double \*pOffset, double \*pSampleRate, int Precision)

**Interface** AgilentPNAPulsed.Application

## ConfigurationFile Method

---

**Description** Recalls an Interface Control file from the hard drive into the analyzer.

**VB Syntax** *IntControl.ConfigurationFile (filename)*

**Variable** **(Type) - Description**

*IntControl* An [InterfaceControl](#) **(object)**

*filename* **(string)** - Full path, file name, and extension (.xml) of the file to recall.  
Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents"

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `IntControl.ConfigurationFile ("C:\Program Files\Agilent\Network Analyzer\Documents\MySettings.xml")`

**C++ Syntax** HRESULT ConfigurationFile(BSTR bstrFile)

**Interface** IInterfaceControl

Write-only

## Continuous Method

---

**Description** The channel continuously responds to trigger signals.

---

**Note:** This command does **NOT** change TriggerSignal to Continuous.

---

**VB Syntax** *chan*.Continuous

**Variable** (Type) - Description

*chan* A Channel (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `chan.Continuous`

**C++ Syntax** HRESULT Continuous()

**Interface** IChannel

**Copy Method**

**Description** Creates a new Cal Set and copies the current Cal Set data into it. Therefore, you now have a clone Cal Set with a different ID. Use this command to manipulate data on a Cal Set without corrupting the original cal data.

**VB Syntax** *CalSet.Copy*

**Variable** (Type) - Description

*CalSet* **(object)** - A Cal Set object

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
Dim mgr As CalManager
Dim ocalset As CalSet
Dim newcalset As CalSet
Set mgr = pna.GetCalManager
'Create a new (empty) Cal Set.
Set ocalset = mgr.CreateCalSet(1)
ocalset.Description = "original calset"
pna.Channel(1).SelectCalSet ocalset.GetGUID, True

'Launch the cal wizard and allow the user to perform the
calibration.
If pna.LaunchCalWizard(False) Then
'If the Launch returns true then the calibration finished.
ocalset.Save

'Copy the Cal Set to the new one.
Set newcalset = ocalset.Copy
newcalset.Description = "copy of original calset"

Else
'If the cal doesn't finish, delete the old Cal Set
'so it isn't taking up unnecessary memory.
mgr.DeleteCalSet ocalset.GetGUID
End If
```

As a result, the programmer can manipulate the data in the new Cal Set and always revert back to the old Cal Set as needed.

**C++ Syntax** HRESULT Copy( ICalSet\*\* pCalSet);

**Interface** ICalSet

Write-only

## CopyToChannel Method

---

**Description** Sets up another channel as a copy of this object's channel.

**VB Syntax** `chan.CopyToChannel(IChanNum)`

**Variable** **(Type) - Description**

*chan* A Channel (**object**)

*IChanNum* (**long integer**) – Number of the channel to become a copy of this channel.

**Return Type** None

**Default** Not Applicable

**Examples** Dim chan As Channel  
Set chan = PNAapp.ActiveChannel  
Const INEW\_CHAN\_NUM As Long = 2  
chan.CopyToChannel(INEW\_CHAN\_NUM)

**C++ Syntax** HRESULT CopyToChannel(long IChanNum);

**Interface** IChannel2



**CreateSParameterEx Method**

---

|                    |                                                                                                                                                                                                                                       |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Creates a new S-Parameter measurement in an existing or new window and specifies the load port for 3-port devices.                                                                                                                    |
| <b>VB Syntax</b>   | <code>app.CreateSParameter chan,recvr,source[,loadPort][,window]</code>                                                                                                                                                               |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                           |
| <i>app</i>         | <u>Application</u> <b>(object)</b>                                                                                                                                                                                                    |
| <i>chan</i>        | <b>(long integer)</b> - Channel number of the new measurement                                                                                                                                                                         |
| <i>recvr</i>       | <b>(long integer)</b> - Port number of the receiver                                                                                                                                                                                   |
| <i>source</i>      | <b>(long integer)</b> - Port number of the source                                                                                                                                                                                     |
| <i>loadPort</i>    | <b>(long integer)</b> - Port number of the load. Required for reflection measurements of 3-port devices on 3-port PNAs.                                                                                                               |
| <i>window</i>      | <b>(long integer)</b> - Optional argument. Window number of the new measurement. Choose 1 to 4. If unspecified, the S-Parameter will be created in the Active Window.                                                                 |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                        |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                        |
| <b>Examples</b>    | <pre>app.CreateSParameter 1,2,1,1 'Creates a new S21 measurement in channel 1 and New window(1) app.CreateSParameter 2,1,1,3,1 'Creates a new S11 measurement on channel 2 with port 3 as the load. Create in the active window</pre> |
| <b>C++ Syntax</b>  | <code>HRESULT CreateSParameter(long ChannelNum, long RcvPort, long SrcPort, long LoadPort, long windowNumber)</code>                                                                                                                  |
| <b>Interface</b>   | IApplication                                                                                                                                                                                                                          |

## CreateCalSet Method

---

**Description** Creates a new Cal Set.

The new cal set is initialized with the stimulus settings from the channel whose number is passed as the argument to this method. Stimulus settings include frequency, bandwidth, number of points, and so forth.

Use this method when you want to manually upload data to the Cal Set using the returned ICal Set interface handle..

The channel number does not restrict the usage of this Cal Set on any other channel. It simply provides a link to the originating channel so that the stimulus values can be stored in the Cal Set.

---

**Note:** Be sure to SAVE the CalSet you are creating. Use [ICalSet::Save](#).

---

**VB Syntax** `calMgr.CreateCalSet (chan)`

**Variable** **(Type) - Description**

`calMgr` **(object)** - A [CalManager](#) object

`chan` **(long)** - channel number of the new Cal Set.

**Return Type** ICal Set Interface

**Default** Not Applicable

**Example** `calMgr.CreateCalSet 1`

**C++ Syntax** HRESULT CreateCalSet( long ChannelNumber, ICal Set\*\* pCal Set);

**Interface** ICalManager

**CreateCustomMeasurementEx Method**

---

**Description** Creates a new custom measurement.

**VB Syntax** `app.CreateCustomMeasurementEx chanNum,ID,initData [,window]`

**Variable** **(Type) - Description**

*app* **(object)** - An Application object

*chanNum* **(long)** -Channel number used by the new measurement; can exist or be a new channel.

*ID* **(string)** - Identifier of the new custom measurement object. The new custom measurement must be installed and registered on the PNA.

Choose from the following Program IDs:

- FCA.VMCMeas
- SMC\_Forward.SMC\_ForwardMeas
- SMC\_Reverse.SMC\_ReverseMeas

*InitData* **(variant)** Measurement specific data for passing initialization data to the new measurement. The variant type and content of the initialization value is defined by the type of measurement being created.

| Program ID                  | Choose from:                                 |
|-----------------------------|----------------------------------------------|
| FCA.VMCMeas                 | "S11"<br>"VC21"<br>"S22"                     |
| SMC_Forward.SMC_ForwardMeas | "S11"<br>"SC21"<br>"S22"<br>"IPwr"<br>"OPwr" |
| SMC_Reverse.SMC_ReverseMeas | "S11"<br>"SC12"<br>"S22"<br>"IPwr"<br>"OPwr" |

*window* **(long)** Optional argument. Number of the window the new custom measurement will be placed in. Choose **1** to **16**. If unspecified, the measurement is placed in the active window.

**Return Type** IMeasurement

**Default** Not Applicable

**Examples** 'To create a forward scalar mixer measurement in channel 2:  
Dim MyMeas as Agilent835x.Measurement  
Set MyMeas = app.CreateCustomMeasurementEx ( 2,  
"SMC\_Forward.SMC\_ForwardMeas", "SC21" )

'To create a reverse scalar mixer measurement in channel 2:  
Dim MyMeas as Agilent835x.Measurement  
Set MyMeas = app.CreateCustomMeasurementEx ( 2,  
"SMC\_Reverse.SMC\_ReverseMeas", "SC12" )

'To create a vector mixer measurement in channel 2:  
Dim MyMeas as Agilent835x.Measurement  
Set MyMeas = app.CreateCustomMeasurementEx ( 2, "FCA.VMCMeas",  
"VC21" )

**C++ Syntax** HRESULT put\_CreateCustomMeasurementEx (long ChannelNum, BSTR guid,  
VARIANT initData, long windowNumber, IMeasurement\*\* ppMeasurement);

**Interface** IApplication3

Write-only

## CreateCustomCal Method

---

**Description** Creates a custom cal object.

**VB Syntax** *calmgr*.CreateCustomCal(*CalType*)

**Variable** (Type) - Description

*calMgr* Cal Manager (Object)

*CalType* **(String)** Name of the calibration. Choose from:

"VMC" or "VectorMixerCal.VMCTYPE"

"SMC" or "ScalarMixerCal.SMCTYPE"

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
Dim CalMgr As ICalManager2
Dim SMC As ISMCTYPE
Set SMC = CreateCustomCal("SMC")
```

See SMC and VMC examples using this command.

**C++ Syntax** HRESULT CreateCustomCal( BSTR CustomCal)

**Interface** ICalManager2

## CreateMeasurement Method

---

**Description** Creates a new measurement

**VB Syntax** `app.CreateMeasurement chanNum,param,IPort[,window]`

**Variable (Type) - Description**

*app* Application (**object**)

*chanNum* (**long**) - Channel number of the new measurement; can exist or be a new channel

*param* (**string**) - New parameter.

**For S-parameters:**

Any S-parameter available in the PNA

For example: "S21"

**For ratioed measurements:**

Any two receivers that are available in the PNA separated with '/'. (See the [block diagram](#) showing the receivers in YOUR PNA.)

For example: "A/R1"

**For non-ratioed measurements:**

Any receiver that is available in the PNA. (See the [block diagram](#) showing the receivers in YOUR PNA.)

For example: "A"

**For Balanced measurements:**

"*topology: Sabxy*"

*topology* - Case insensitive. Choose from:

- **sbal** - single-ended to balanced
- **ssb** - single-ended / single-ended to balanced
- **bbal** - balanced to balanced

**Sabxy** -

**Where**

**a** = output mode

**b** = input mode

(choose from the following for both a and b:)

- **d** - differential
- **c** - common
- **s** - single ended

**x** = output logical port number

**y** = input logical port number

*I*Port **(long)** -

**Load port** if *param* is a reflection S-Parameter.

**Ignored** if *param* is a transmission S-Parameter or balanced parameter.

**Source port** if *param* is ratioed or unratioed measurement.

*window* **(long)** Optional argument. Window number of the new measurement. Choose **1** to **16**. If unspecified, the measurement will be created in the Active Window.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.CreateMeasurement(1, "A/R1", 1, 0)`

`app.CreateMeasurement(1, "bbal:Sdd21", 1)`

**C++ Syntax** HRESULT CreateMeasurement(long ChannelNum, BSTR strParameter, long IPort, long windowNumber)

**Interface** IApplication

## DataToMemory Method

---

|                    |                                                                                                                                                             |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Stores the active measurement data into memory creating a memory trace. The memory can then be displayed or used in calculations with the measurement data. |
| <b>VB Syntax</b>   | <i>meas</i> .DataToMemory                                                                                                                                   |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                 |
| <i>meas</i>        | A Measurement ( <b>object</b> )                                                                                                                             |
| <b>Return Type</b> | Not Applicable                                                                                                                                              |
| <b>Default</b>     | Not Applicable                                                                                                                                              |
| <b>Examples</b>    | <code>meas.DataToMemory</code>                                                                                                                              |
| <b>C++ Syntax</b>  | HRESULT DataToMemory()                                                                                                                                      |
| <b>Interface</b>   | IMeasurement                                                                                                                                                |



Write-only

## Delete Method

---

**Description** Deletes the measurement.

**VB Syntax** *meas.Delete*

**Variable** (Type) - Description

*meas* The Measurement object to delete (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `meas.Delete`

**C++ Syntax** HRESULT Delete()

**Interface** IMeasurement

Write-only

## DeleteMarker Method

---

**Description** Deletes a marker from the measurement.

**VB Syntax** *meas.DeleteMarker(Mnum)*

**Variable** (Type) - Description

*meas* A Measurement (**object**)

*Mnum* (**long**) - Any existing marker number in the measurement

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `meas.DeleteMarker(1)`

**C++ Syntax** HRESULT DeleteMarker(long IMarkerNumber)

**Interface** IMeasurement

## DeleteAllMarkers Method

---

**Description** Deletes all of the markers from the measurement.

**VB Syntax** *meas.DeleteAllMarkers*

**Variable** (Type) - Description

*meas* **(object)** - The Measurement object from which markers will be deleted.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `meas.DeleteAllMarkers`

**C++ Syntax** HRESULT DeleteAllMarkers()

**Interface** IMeasurement

**DeleteCalSet Method**

---

**Description** Deletes a Cal Set from the set of available Cal Sets. This method immediately updates the Cal Set file on the hard drive. If the Cal Set is currently being used by a channel, this request will be denied and an error is returned.

Errors returned by this method:

```
E_NA_CAL_SET_IN_USE
E_NA_Cal Set_NOT_FOUND
E_NA_Cal Set_SAVE_FAILED
```

Using the [Cal Sets collection](#) is a convenient way to manage Cal Sets.

**VB Syntax** *calMgr.DeleteCalSet (GUID)*

**Variable** **(Type) - Description**

*calMgr* **(object)** - A CalManager object

*GUID* **(string)** - GUID number of the Cal Set to be deleted

**Return Type** Not Applicable

**Default** Not Applicable

**Example**

```
dim cs As CalSet ' the collection
dim strGUID as string

strGUID = cs.GetGUID
calMgr.DeleteCalSet strGUID
```

**C++ Syntax** HRESULT DeleteCalSet( BSTR strGUID);

**Interface** ICalManager

## DeleteShortCut Method

---

**Description** Removes a macro from the list of macros in the analyzer. Does not remove the file.

**Note:** There are always 12 macro positions. They do not have to be sequential. For example, you can have number 7 but no numbers 1 to 6.

---

**VB Syntax** `app.DeleteShortCut item`

**Variable** **(Type) - Description**

`app` An Application (**object**)

`item` (**long integer**) number of the macro to be deleted.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.DeleteShortCut 2`

**C++ Syntax** HRESULT DeleteShortcut(long Number )

**Interface** IApplication

## DisallowAllEvents Method

---

**Description** Sets event filtering to monitor NO eventst.

**VB Syntax** `app.DisallowAllEvents`

**Variable** (Type) - Description

`app` An Application (**object**)

**Return  
Type** Not Applicable

**Default** Not Applicable

**Examples** `app.DisallowAllEvents`

**C++ Syntax** HRESULT DisallowAllEvents()

**Interface** IApplication

Write-only

## DoPrint Method

---

**Description** Prints the screen to the default Printer.

**VB Syntax** *app.DoPrint*

**Variable** (Type) - Description

*app* An Application (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.DoPrint`

**C++ Syntax** HRESULT DoPrint()

**Interface** IApplication

## DoECAL1PortEx Method

---

**Description** This method replaces [DoECAL1Port Method](#).  
 Does a 1-Port calibration using an ECAL module. You must first have a 1-port measurement active to perform the calibration.  
 The characterization within the ECal module that will be used for the calibration is specified by [ECALCharacterizationEx](#). The default value is 0.

**VB Syntax** `cal.DoECAL1PortEx [port][,module]`

---

### Variable (Type) - Description

`cal` A Calibrator (**object**)

`port` (**long integer**) Optional argument - Port number to calibrate. Choose from:  
 1 - Calibrate port 1 (default if unspecified)  
 2 - Calibrate port 2

`module` (**long integer**) Optional argument. ECal module.

Choose from modules **1** through **8**

Use [IsECALModuleFoundEx](#) to determine the number of modules connected to the PNA

Use [GetECALModuleInfoEx](#) to returns the model and serial number of each module.

**Return Type** None

**Default** Not Applicable

---

**Examples** `cal.DoECAL1PortEx, 2, 2`

---

**C++ Syntax** `HRESULT DoECAL1PortEx(long port, long moduleNumber = 1);`

**Interface** ICalibrator4



## DoECAL2PortEx Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                             |
|--------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p>This method replaces <a href="#">DoECAL2Port Method</a>.</p> <p>Does a 2-Port calibration using an ECAL module. You must first have a 2-port measurement active to perform the calibration.</p> <p>The characterization within the ECal module that will be used for the calibration is specified by <a href="#">ECALCharacterizationEx</a>. The default value is 0.</p> |
| <b>VB Syntax</b>   | <code>cal.DoECAL2PortEx [portA][,portB][,module]</code>                                                                                                                                                                                                                                                                                                                     |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                 |
| <i>cal</i>         | A Calibrator ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                              |
| <i>portA</i>       | <p><b>(long integer)</b> Optional argument - Number of the receive port to calibrate. Choose from:</p> <ul style="list-style-type: none"> <li>1 - Calibrate port 1 (default, if unspecified)</li> <li>2 - Calibrate port 2</li> <li>3 - Calibrate port 3 (if the PNA has 3 ports)</li> </ul>                                                                                |
| <i>portB</i>       | <p><b>(long integer)</b> Optional argument - Number of the source port to calibrate. Choose from:</p> <ul style="list-style-type: none"> <li>1 - Calibrate port 1 (default, if unspecified)</li> <li>2 - Calibrate port 2</li> <li>3 - Calibrate port 3 (if the PNA has 3 ports)</li> </ul>                                                                                 |
| <i>module</i>      | <p><b>(long integer)</b> Optional argument. ECal module.</p> <p>Choose from modules <b>1</b> through <b>8</b></p> <p>Use <a href="#">IsECALModuleFoundEx</a> to determine the number of modules connected to the PNA</p> <p>Use <a href="#">GetECALModuleInfoEx</a> to returns the model and serial number of each module.</p>                                              |
| <b>Return Type</b> | None                                                                                                                                                                                                                                                                                                                                                                        |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                              |
| <b>Examples</b>    | <code>cal.DoECAL2PortEx,1,2,3</code>                                                                                                                                                                                                                                                                                                                                        |
| <b>C++ Syntax</b>  | <code>HRESULT DoECAL2PortEx( long portA = 1, long portB =2, long moduleNumber = 1);</code>                                                                                                                                                                                                                                                                                  |
| <b>Interface</b>   | ICalibrator4                                                                                                                                                                                                                                                                                                                                                                |

## DoneCalConfidenceCheckECAL Method

---

**Description** Concludes the Confidence Check and sets the ECal module back into the idle state.

**VB Syntax** *cal*.DoneCalConfidenceCheckECAL

**Variable** (Type) - Description

*cal* A Calibrator (**object**)

**Return Type** None

**Default** None

**Examples** *cal*.DoneCalConfidenceCheckECAL

**C++ Syntax** HRESULT DoneCalConfidenceCheckECAL( );

**Interface** ICalibrator

**DoReceiverPowerCal Method**

---

|                    |                                                                                                                                                                                                                                                                              |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This command replaces <u>DataToDivisor</u> , <u>LogMagnitudeOffset</u> , <u>Normalization</u> , <u>InterpolateNormalization</u> .<br>Performs a receiver power calibration.                                                                                     |
| <b>VB Syntax</b>   | <code>cal.DoReceiverPowerCal(param, srcPort [,pwrOffset])</code>                                                                                                                                                                                                             |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                  |
| <i>cal</i>         | A <u>Calibrator</u> ( <b>object</b> )                                                                                                                                                                                                                                        |
| <i>param</i>       | <b>(string)</b> – Receiver to be calibrated.<br>Choose from: <b>A   B   R   R1   R2</b><br><b>C   R3</b> - For 3-port and 4-port analyzers only.<br><b>D   R4</b> - For 4-port analyzers only.                                                                               |
| <i>srcPort</i>     | <b>(long integer)</b> – Number of the port which will supply source power to the receiver during this cal.                                                                                                                                                                   |
| <i>pwrOffset</i>   | <b>(double)</b> – Optional argument. Offset value in dB. Adjusts a receiver power cal to account for components or adapters that are added between the source port and receiver while performing this cal. Specify loss as a negative number; and gain as a positive number. |
| <b>Return Type</b> | None                                                                                                                                                                                                                                                                         |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                               |
| <b>Examples</b>    | <code>cal.DoReceiverPowerCal "B", 1, -10</code>                                                                                                                                                                                                                              |
| <b>C++ Syntax</b>  | <code>HRESULT DoReceiverPowerCal(BSTR parameter, long lSrcPort, double dPowerOffset);</code>                                                                                                                                                                                 |
| <b>Interface</b>   | ICalibrator5                                                                                                                                                                                                                                                                 |

Read-only

## Execute Method

---

**Description** This method can be used with SCPI command :SYST:ERR? to convert scpi errors into text.

**VB Syntax** Scpi.**Execute**(SCPI\_Command As String)

**Variable** **(Type) - Description**

*scpi* A ScpiStringParser **(Object)**

*SCPI\_Command* **(String)** - Any valid SCPI command

**Return Type** String

**Default** Not Applicable

**Examples**

```
Dim scpi As ScpiStringParser
Set scpi = app.ScpiStringParser
scpi.Execute("SYST:PRES");
ErrorString = scpi.Execute("SYST:ERRor?");
```

**C++ Syntax** Execute([in] BSTR SCPI\_Command,[out,retval] BSTR \* pQueryResponse);

**Interface** IScpiStringParser2

**ExecuteShortcut Method**

---

|                    |                                                                                                                                                                                                   |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Executes a Macro (shortcut) stored in the analyzer. Use <a href="#">app.getShortcut</a> to list existing macros. Use <a href="#">app.putShortcut</a> to associate the macro number with the file. |
| <b>VB Syntax</b>   | <i>app.ExecuteShortcut index</i>                                                                                                                                                                  |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                       |
| <i>app</i>         | An <a href="#">Application</a> ( <b>object</b> )                                                                                                                                                  |
| <i>index</i>       | <b>(long integer)</b> - Number of the macro stored in the analyzer.                                                                                                                               |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                    |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                    |
| <b>Examples</b>    | <code>app.ExecuteShortcut 1</code>                                                                                                                                                                |
| <b>C++ Syntax</b>  | HRESULT ExecuteShortcut(long index)                                                                                                                                                               |
| <b>Interface</b>   | IApplication                                                                                                                                                                                      |

## GenerateErrorTerms Method

---

**Description** Generates the error terms for the specified calibration type, stores the error terms in a Cal Set, saves the Cal Set, and returns the Cal Set GUID.

If ALL the data for the cal type has NOT been acquired an error message is returned.

**VB Syntax** *value* = *obj*.**GenerateErrorTerms**

**Variable** **(Type) - Description**

*value* (String) - Variable to store the returned GUID or error message.

*obj* Any of the following:

GuidedCalibration (object)

SMCType (object)

VMCType (object)

**Return Type** String

**Default** Not Applicable

**Examples** `string = SMC.GenerateErrorTerms`

**C++ Syntax** HRESULT put\_GenerateErrorTerms(BSTR\* calsetGUID);

**Interface** IGuidedCalibration

SMCType

VMCType

## GenerateSteps Method

---

**Description** Returns the number of steps required to complete the calibration type.

**VB Syntax** `value = obj.GenerateSteps`

**Variable** **(Type) - Description**

*value* (long) - Variable to store the returned number of steps

*obj* Any of the following:

GuidedCalibration (object)

SMCType (object)

VMCType (object)

**Return Type** Long

**Default** Not Applicable

**Examples** `value = SMC.GenerateSteps`

**C++ Syntax** `HRESULT put_GenerateSteps(long* steps);`

**Interface** IGuidedCalibration

SMCType

VMCType

Read-only

## GetAuxIO Method

---

**Description** This method returns the IAuxIO interface.

**VB Syntax** `app.GetAuxIO`

**Variable** (Type) - Description

`app` An Application (**object**)

**Return Type** IHWAuxIO

**Default** Not Applicable

**Example**

```
Dim app As AgilentPNA835x.Application
Dim aux As HWAuxIO
Set aux = app.GetAuxIO
```

**C++ Syntax** HRESULT GetAuxIO (IHWAuxIO \*\*pAux);

**Interface** IApplication



Write-only

## GetCalStandard Method

---

**Description** Returns a handle to a calibration standard for modifying its definitions. To select a standard for performing a calibration (use `Calibrator.AcquireCalStandard`).

**VB Syntax** `calkit.GetCalStandard(index)`

**Variable** **(Type) - Description**

*calkit* A calKit (**object**)

*index* (**long**) - Number of calibration standard. Choose **1** to **30**; (there are 30 cal standards in every kit).

**Return Type** calStandard

**Default** Not Applicable

**Examples**

```
Dim short As CalStandard
Set short = calKit.getCalStandard(1)
short.label = "myShort"
```

**C++ Syntax** HRESULT GetCalStandard(long standardNumber, ICalStandard \*\*pCalStd)

**Interface** ICalKit

## GetCalManager Method

---

**Description** This method returns the [ICalManager](#) interface.

**VB Syntax** `app.GetCalManager`

**Variable** **(Type) - Description**

`app` An [Application](#) (**object**)

**Return Type** ICalManager\*

**Default** Not Applicable

**Example**

```
dim app as AgilentPNA835x.Application
dim mgr as CalManager
set mgr = app.GetCalManager
```

**C++ Syntax** HRESULT GetCalManager( ICalManager \*\*mgr);

**Interface** IApplication

## Get CalSetByGUID Method

---

**Description** Requests a Cal Set by GUID. Returns an ICal Set interface.

**VB Syntax** *calMgr*.**GetCalSetByGUID** (*GUID*)

**Variable** **(Type) - Description**

*calMgr* **(object)** - A CalManager object

*GUID* **(string)** - GUID of the Cal Set being requested.

**Return Type** Interface object

**Default** Not Applicable

**Example** `calMgr.GetCalSetByGUID (2B893E7A-971A-11d5-8D6C-00108334AE96)`

**C++ Syntax** HRESULT GetCalSetByGUID( BSTR\* strGUID, ICal Set\* pCalSet);

**Interface** ICalManager

## GetCalSetCatalog Method

---

**Description** Returns a string containing a list of comma-separated GUIDs in the following format:

```
{FD6F863E-9719-11d5-8D6C-00108334AE96},
{1B03B2CE-971A-11d5-8D6C-00108334AE96},
{2B893E7A-971A-11d5-8D6C-00108334AE96}
```

**VB Syntax** *value* = *calMgr*.**GetCalSetCatalog**

**Variable** **(Type) - Description**

*value* **(string)** - Variable to store the returned GUID list

*calMgr* **(object)** - A CalManager object

**Return Type** String

**Default** Not Applicable

**Example** `value = calMgr.GetCalSetCatalog`

**C++ Syntax** HRESULT GetCalSetCatalog( BSTR);

**Interface** ICalManager

## GetCalSetUsageInfo Method

---

- Description** Returns a string identifying the Cal Set currently in use by the specified channel.
- This method identifies the Cal Set being used by returning its GUID.
- This method also identifies the "Error Term set" within the Cal Set.
- Error term sets are identified by integers, with set 0 belonging to the original (non-interpolated) terms. As stimulus values for a channel are changed causing interpolation to be required, a new Error Term set is constructed within the Cal Set to hold the interpolated Error Terms. The sets are sequentially numbered 1, 2, 3, and so forth. These Error Term sets are destroyed when they are no longer being used.
- If there is no Cal Set in use for the given channel, the <GUID> argument is set to the empty string.
- VB Syntax** `calMgr.GetCalSetUsageInfo (chan, GUID, setNumber)`
- Variable (Type) - Description**
- calMgr* **(object)** - A CalManager object
- chan* **(long [in])** - channel of the Cal Set being requested
- GUID* **(string [out])** - variable to store the GUID of the Cal Set being requested. If there is no Cal Set in use for the given channel, the <GUID> argument is set to the empty string.
- setNumber* **(long [out])** - variable to store the error term ID being requested. If the returned argument is greater than 0, the set is being interpolated.
- Return Type** String , Long Integer
- Default** Not Applicable
- Example** `calMgr.GetCalSetUsageInfo (1, GUID, EtermID)`
- C++ Syntax** HRESULT GetCalSetUsageInfo (long IChannel, BSTR\* CalSetGUID, long\* etermSetID);
- Interface** ICalManager

Read only

## GetCalTypes

---

**Description** Returns a list of available calibration types, both Standard and Custom. The Standard CalTypes are the same on all PNA's, but the Custom CalTypes are not necessarily the same. They are dependent on the custom components that have been installed in the instrument.

**VB Syntax** `v = CalManager.GetCalTypes`

**Variable** (Type) - Description

v NameGuidPair: contains the calibration type name and associated GUID for each cal type known to the PNA

**Return Type** **(variant)** of type VT\_ARRAY. The array is two dimensional containing elements of type variant.

**Default** Not Applicable

**Examples** `v =CalManager.GetCalTypes`

**C++ Syntax** HRESULT GetCalTypes( VARIANT \* NameGuidPair )

**Interface** ICalManager2

Read-only

**GetComplex Method**

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                  |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Retrieves complex data from the specified location.<br>See also <a href="#">getNAComplex</a> , <a href="#">getData</a> , and <a href="#">getPairedData</a> Methods                                                                                                                                                                                                               |
| <b>VB Syntax</b>   | <i>measData</i> . <b>getComplex</b> <i>location, numPts, real(), imag()</i>                                                                                                                                                                                                                                                                                                      |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                      |
| <i>measData</i>    | An IArrayTransfer interface which supports the Measurement object                                                                                                                                                                                                                                                                                                                |
| <i>location</i>    | <b>(enum NADataStore - IArrayTransfer)</b> - Where the data you want is residing. Choose from:<br>0 - naRawData<br>1 - naCorrectedData<br>2 - naMeasResult<br>3 - naRawMemory<br>4 - naMemoryResult<br>5 - naDivisor - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using <a href="#">DataToDivisor Method</a> . |
| <i>numPts</i>      | <b>(long integer)</b> - Number of data points requested<br>[out] - specifies number of data elements returned<br>[in] - specifies the data being requested or the capacity of the arrays                                                                                                                                                                                         |
| <i>real</i>        | <b>(single)</b> - Array to store the real values                                                                                                                                                                                                                                                                                                                                 |
| <i>imag</i>        | <b>(single)</b> - Array to store the imaginary values                                                                                                                                                                                                                                                                                                                            |
| <b>Return Type</b> | Single                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                   |
| <b>Examples</b>    | <pre>Dim real(201) AS Single Dim imag(201) AS Single Dim pts as Integer Dim measData As IArrayTransfer Set measData = app.ActiveMeasurement measData.getComplex naCorrectedData, pts, real(0), imag(0)</pre>                                                                                                                                                                     |
| <b>C++ Syntax</b>  | IArrayTransfer - HRESULT getComplex(tagNADataStore DataStore, long* pNumValues, float* pReal, float* plmag)                                                                                                                                                                                                                                                                      |
| <b>Interface</b>   | IArrayTransfer                                                                                                                                                                                                                                                                                                                                                                   |

Read-only

**getDataByString Method**

---

**Description** Retrieves variant data from the specified location in your choice of formats.

**VB Syntax** `data = meas.getDataByString location, format`

**Variable** **(Type) - Description**

`data` **(variant)** - Array to store the data.

`meas` **(object)** - A Measurement object

`location` **(string)** – Name of the buffer to be read. Choose from:

"naRawData"

"naCorrectedData"

"naMeasResult"

"naRawMemory"

"naMemoryResult"

"naDivisor" - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using [DataToDivisor Method](#).

`format` **(enum NADataFormat)** - Format in which you would like the data. It does not have to be the displayed format. Choose from:

0 - naDataFormat\_LinMag

1 - naDataFormat\_LogMag

2 - naDataFormat\_Phase

**3 - naDataFormat\_Polar \***

**4 - naDataFormat\_Smith \***

5 - naDataFormat\_Delay

6 - naDataFormat\_Real

7 - naDataFormat\_Imaginary

8 - naDataFormat\_SWR

\* **Specfiy Smith or Polar** formats to obtain complex data pairs, which require a two-dimensional array **varData (numpts, 2)** to accomodate both real and imaginary data.

All scalar formats return a single dimension **varData(numpts)**.

**Return Type** Variant array

**Default** Not Applicable

**Examples** `meas.getDataByString "VectorResult0", naDataFormat_Phase`

**C++ Syntax** HRESULT getDataByString( BSTR location, tagDataFormat dataFormat, VARIANT \* pData );



**Interface** IMeasurement

## GetData Method

---

**Description** Retrieves variant data from the specified location in your choice of formats. To get smoothed data from any of the specified locations, the format must be the same as the displayed format.

**Note:** This method returns a variant which is less efficient than methods available on the [IArrayTransfer](#) interface.

**Note:** If you plan to **Put** this data back into analyzer, [putDataComplex](#) (variant data) method requires complex, two-dimensional data. Therefore, request the data in **Polar** format.

**VB Syntax** `data = meas.GetData location, format`

**Variable** **(Type) - Description**

*data* Variant array to store the data.

*meas* A Measurement (**object**)

*location* (**enum NADataStore**) - Where the data you want is residing. Choose from:

0 - naRawData

1 - naCorrectedData

2 - naMeasResult

3 - naRawMemory

4 - naMemoryResult

5 - naDivisor When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using [DataToDivisor Method](#).

*format* (**enum NADataFormat**) - Format in which you would like the data. It does not have to be the displayed format. Choose from:

0 - naDataFormat\_LinMag

1 - naDataFormat\_LogMag

2 - naDataFormat\_Phase

**3 - naDataFormat\_Polar \***

**4 - naDataFormat\_Smith \***

5 - naDataFormat\_Delay

6 - naDataFormat\_Real

7 - naDataFormat\_Imaginary

8 - naDataFormat\_SWR

\* **Specify Smith or Polar** formats to obtain complex data pairs, which require a two-dimensional array **varData (numpts, 2)** to accommodate both real and imaginary data.

All scalar formats return a single dimension **varData(numpts)**.

**naDataFormat\_Phase** returns degrees. However, [putDataScalar](#) method accepts data in radians (not degrees) and displays in degrees.

**Return Type** Variant array - automatically dimensioned to the size of the data

**Default** Not Applicable

**Examples**

```
Dim varData As Variant
varData = meas.GetData(naMeasResult,naDataFormat_Phase)
'Print Data
For i = 0 to chan.NumberOfPoints-1
 Print varData(i)
Next i
```

**C++ Syntax** HRESULT getData(tagNADataStore DataStore, tagDataFormat DataFormat, VARIANT \*pData)

**Interface** IMeasurement

Read-only

## GetECALModuleInfoEx Method

---

**Description** This property replaces [Get ECALModuleInfo Method](#).

Returns the following information about the connected ECAL module: model number, serial number, connector type, calibration date, min and max frequency.

The characterization within the ECal module that this information will be read from is specified by [ECALCharacterizationEx](#). The default value is 0.

**VB Syntax** `moduleInfo = cal.GetECALModuleInfoEx (module)`

**Variable** **(Type) - Description**

`moduleInfo` **(string)** - variable to store the module information

`cal` A Calibrator **(object)**

`module` **(long integer)** ECal module.

Choose from modules **1** through **8**

Use [IsECALModuleFoundEx](#) to determine the number of modules connected to the PNA

**Return Type** String

**Default** Not Applicable

**Examples** `info = cal.GetECALModuleInfoEx(2)`

**Example return string:**

```
ModelNumber: 85092-60007, SerialNumber: 01386, ConnectorType:
N5FN5F, PortAConnector: Type N (50) female, PortBConnector: Type
N (50) female, MinFreq: 30000, MaxFreq: 9100000000,
NumberOfPoints: 250, Calibrated: July 4 2002
```

**C++ Syntax** `HRESULT GetECALModuleInfoEx(long moduleNumber, BSTR* info);`

**Interface** ICalibrator4

**GetErrorTerm Method - OBSOLETE**

**Description** **Note:** This command is replaced by [Get ErrorTermByString Method](#)

Retrieves error term data that is used for error correction. The data is complex pairs. Memory for the returned Variant is allocated by the server. The server returns a variant containing a two-dimensional safe Array.

This method returns a variant which is less efficient than [getErrorTermComplex](#) on the ICalData interface.

[Learn about reading and writing Calibration data.](#)

**VB Syntax** `data = cal.getErrorTerm term, rcv, src`

**Variable (Type) - Description**

`data` Variant array to store the data.

`cal` A Calibrator (**object**)

`term` (**enum As NaErrorTerm**). Choose from:

naErrorTerm\_Directivity\_Isolation

naErrorTerm\_Match

naErrorTerm\_Tracking

`rcv` (**long integer**) - Receiver Port

`src` (**long integer**) - Source Port

| To get this             | Specify these parameters:  |            |            |
|-------------------------|----------------------------|------------|------------|
| Error Term              | <i>term</i>                | <i>rcv</i> | <i>src</i> |
| Fwd Directivity         | naET_Directivity Isolation | 1          | 1          |
| Rev Directivity         | naET_Directivity Isolation | 2          | 2          |
| Fwd Isolation           | naET_Directivity Isolation | 2          | 1          |
| Rev Isolation           | naET_Directivity Isolation | 1          | 2          |
| Fwd Source Match        | naErrorTerm_Match          | 1          | 1          |
| Rev Source Match        | naErrorTerm_Match          | 2          | 2          |
| Fwd Load Match          | naErrorTerm_Match          | 2          | 1          |
| Rev Load Match          | naErrorTerm_Match          | 1          | 2          |
| Fwd Reflection Tracking | naErrorTerm_Tracking       | 1          | 1          |
| Rev Reflection Tracking | naErrorTerm_Tracking       | 2          | 2          |
| Fwd Trans Tracking      | naErrorTerm_Tracking       | 2          | 1          |
| Rev Trans Tracking      | naErrorTerm_Tracking       | 1          | 2          |

---

**Return Type** Variant

**Default** Not Applicable

**Examples** `Dim varError As Variant  
varError = cal.getErrorTerm(naErrorTerm_Tracking,2,1)`

**C++ Syntax** HRESULT getErrorTerm(tagNAErrorTerm ETerm, long ReceivePort, long SourcePort, VARIANT\* pData)

**Interface** ICalibrator

**GetErrorTerm Method OBSOLETE**


---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p>This command has been replaced with <a href="#">GetErrorTermByString</a></p> <hr/> <p>Returns error term data from the Cal Set. The returned data is complex pairs.</p> <p>Learn more about <a href="#">Reading and Writing Cal Data</a></p> <p>See examples of <a href="#">Reading</a> and <a href="#">Writing</a> Cal Set Data</p>                                                                                                                                                                                                     |
| <b>VB Syntax</b>   | <code>data = calSet.getErrorTerm (setNumber, term, rcv, src)</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <i>data</i>        | <p><b>(Variant)</b> Two-dimensional safe array to store the returned data. Memory for the returned Variant is allocated by the PNA and must be released by client.</p> <hr/> <p><b>Note:</b> See also <a href="#">getErrorTermComplex</a> on the ICalData2 interface to avoid using the variant data type.</p>                                                                                                                                                                                                                              |
| <i>calSet</i>      | A <a href="#">Cal Set</a> ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <i>setNumber</i>   | <p><b>(Long)</b> There can be more than one set of error terms in a Cal Set.</p> <ul style="list-style-type: none"> <li>• SetNumber <b>0</b> contains the original set of error terms for a Cal Set.</li> <li>• SetNumbers <b>&gt; 0</b> contain Interpolated error terms. Interpolated error terms are generated when interpolation is required and destroyed when no longer used. <a href="#">Learn about Interpolation.</a></li> <li>• To determine the SetNumber in use by a channel, see <a href="#">GetCalSetUsageInfo</a></li> </ul> |
| <i>term</i>        | <p><b>(enum As NaErrorTerm2).</b> Choose from:</p> <p>0 - naET_Directivity (rcv = src)</p> <p>1 - naET_SourceMatch (rcv = src)</p> <p>2 - naET_ReflectionTracking (rcv = src)</p> <p>3 - naET_TransmissionTracking (rcv ≠ src)</p> <p>4 - naET_LoadMatch (rcv ≠ src)</p> <p>5 - naET_Isolation (rcv ≠ src)</p>                                                                                                                                                                                                                              |
| <i>rcv</i>         | <b>(Long)</b> - Receiver Port                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <i>src</i>         | <b>(Long)</b> - Source Port                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Return Type</b> | Variant                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Examples</b>    | <pre>Dim varError As Variant varError = CalSet.getErrorTerm(0,naET_TransmissionTracking,2,1)</pre>                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <b>C++ Syntax</b>  | HRESULT getErrorTerm(long setID, tagNAErrorTerm2 ETerm, long ReceivePort, long SourcePort, VARIANT* pData)                                                                                                                                                                                                                                                                                                                                                                                                                                  |

**Interface** ICalSet



## GetErrorTermByString Method

---

**Description** Returns error term data from the Cal Set by specifying the string name of the error term.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

**VB Syntax** `pdata = calset.GetErrorTermByString(setNumber, errorTerm)`

**Variable (Type) - Description**

*pdata* **(Variant)** Two-dimensional safe array to store the returned data. Memory for the returned Variant is allocated by the PNA and must be released by client.

**Note:** See also [getErrorTermComplexByString](#) on the ICalData3 interface to avoid using the variant data type.

---

*calset* A [Cal Set \(object\)](#)

*setNumber* **(Long)** There can be more than one set of error terms in a Cal Set.

- SetNumber **0** contains the original set of error terms for a Cal Set.
- SetNumbers **> 0** contain Interpolated error terms. Interpolated error terms are generated when interpolation is required and destroyed when no longer used. [Learn about Interpolation](#).
- To determine the SetNumber in use by a channel, see [GetCalSetUsageInfo](#)

*errorTerm* **(String)** The string name used to identify a particular error term in the Cal Set. An example string for port 3 directivity in a full 2 port cal might be "Directivity(3,3)". To determine the string names of error terms, see [GetErrorTermList2](#).

**Return Type** Variant

**Default** Not Applicable

**Examples** [See an Example](#)

**C++ Syntax** HRESULT GetErrorTermByString (long SetNumber, BSTR bufferName, VARIANT\* pdata);

**Interface** ICalSet2

**GetErrorTermComplex Method OBSOLETE**

---

**Description** This command has been replaced by [Get ErrorTermComplexByString](#).  
Retrieves error term data from the error correction buffer. The data is in complex pairs.  
Learn more about [reading and writing Cal Data using COM](#).  
This method exists on a non-default interface. If you cannot access this method, use the [GetErrorTerm](#) Method on ICalibrator.

**VB Syntax** *eData*.**GetErrorTermComplex** *term, rcv, src, numPts, real(), imag()*

**Variable** **(Type) - Description**

*eData* An ICalData pointer to the Calibrator object

*term* **(enum NAErrorTerm)** - The error term to be retrieved. Choose from:

- **naErrorTerm\_Directivity\_Isolation**
- **naErrorTerm\_Match**
- **naErrorTerm\_Tracking**

*rcv* **(long integer)** - Receiver Port

*src* **(long integer)** - Source Port

*numPts* **(long integer)** - on input, max number of data points to return; on output: indicates the actual number of data points returned.

*real()* **(single)** - array to accept the **real** part of the error-term. One-dimensional for the number of data points.

*imag()* **(single)** - array to accept the **imaginary** part of the error-term. One-dimensional for the number of data points.

---

|                    | To get this                                                                                                                                                                               | Specify these parameters:  |            |            |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------|------------|------------|
|                    | Error Term                                                                                                                                                                                | <i>term</i>                | <i>rcv</i> | <i>src</i> |
|                    | Fwd Directivity                                                                                                                                                                           | naET_Directivity Isolation | 1          | 1          |
|                    | Rev Directivity                                                                                                                                                                           | naET_Directivity Isolation | 2          | 2          |
|                    | Fwd Isolation                                                                                                                                                                             | naET_Directivity Isolation | 2          | 1          |
|                    | Rev Isolation                                                                                                                                                                             | naET_Directivity Isolation | 1          | 2          |
|                    | Fwd Source Match                                                                                                                                                                          | naErrorTerm_Match          | 1          | 1          |
|                    | Rev Source Match                                                                                                                                                                          | naErrorTerm_Match          | 2          | 2          |
|                    | Fwd Load Match                                                                                                                                                                            | naErrorTerm_Match          | 2          | 1          |
|                    | Rev Load Match                                                                                                                                                                            | naErrorTerm_Match          | 1          | 2          |
|                    | Fwd Reflection Tracking                                                                                                                                                                   | naErrorTerm_Tracking       | 1          | 1          |
|                    | Rev Reflection Tracking                                                                                                                                                                   | naErrorTerm_Tracking       | 2          | 2          |
|                    | Fwd Trans Tracking                                                                                                                                                                        | naErrorTerm_Tracking       | 2          | 1          |
|                    | Rev Trans Tracking                                                                                                                                                                        | naErrorTerm_Tracking       | 1          | 2          |
| <b>Return Type</b> | Single                                                                                                                                                                                    |                            |            |            |
| <b>Default</b>     | Not Applicable                                                                                                                                                                            |                            |            |            |
| <b>Examples</b>    | <pre> ReDim rel(numpts) ReDim img(numpts) Dim eData As ICalData Set eData = chan.Calibrator eData.getErrorTermComplex naErrorTerm_Directivity_Isolation, 1, 1, 201, rel(0), img(0) </pre> |                            |            |            |
| <b>C++ Syntax</b>  | HRESULT raw_getErrorTermComplex(tagNAErrorTerm ETerm, long ReceivePort, long SourcePort, long* pNumValues, float* pReal, float* plmag)                                                    |                            |            |            |
| <b>Interface</b>   | ICalData                                                                                                                                                                                  |                            |            |            |

**GetErrorTermComplex Method** OBSOLETE

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p>This command is <u>replaced</u> with <u>Get ErrorTermComplexByString</u></p> <hr/> <p>Returns error term data from the Cal Set. The data is in complex pairs.</p> <p>Learn more about <u>Reading and Writing Cal Data</u></p> <p>See examples of <u>Reading</u> and <u>Writing</u> Cal Set Data</p> <hr/> <p><b>Note:</b> This method exists on a non-default interface. If you cannot access this method, use the <u>GetErrorTerm</u> Method on ICal Set.</p> <hr/>                                                                        |
| <b>VB Syntax</b>   | <i>iCalData2</i> . <b>GetErrorTermComplex</b> <i>setNumber, term, rcv, src, numPts, real(), imag()</i>                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
| <i>iCalData2</i>   | An <u>ICalData2</u> pointer to the Cal Set object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <i>setNumber</i>   | <p><b>(Long)</b> There can be more than one set of error terms in a Cal Set.</p> <ul style="list-style-type: none"> <li>• <i>setNumber</i> <b>0</b> contains the original set of error terms for a Cal Set.</li> <li>• <i>setNumbers</i> <b>&gt; 0</b> contain Interpolated error terms. Interpolated error terms are generated when interpolation is required and destroyed when no longer used. <u>Learn about Interpolation.</u></li> <li>• To determine the <i>setNumber</i> in use by a channel, see <u>GetCalSetUsageInfo</u></li> </ul> |
| <i>term</i>        | <p><b>(enum NAEErrorTerm2)</b> - The error term to be retrieved. Choose from:</p> <p>0 - naET_Directivity</p> <p>1 - naET_SourceMatch</p> <p>2 - naET_ReflectionTracking</p> <p>3 - naET_TransmissionTracking</p> <p>4 - naET_LoadMatch</p> <p>5 - naET_Isolation</p>                                                                                                                                                                                                                                                                          |
| <i>rcv</i>         | <b>(Long)</b> - Receiver Port                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <i>src</i>         | <b>(Long)</b> - Source Port                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
| <i>numPts</i>      | <p><b>(Long)</b> An In/Out parameter.</p> <p>On the way <b>in</b>, you specify the <b>max</b> number of values being requested.</p> <p>On the way <b>out</b>, the PNA returns number of values actually returned.</p>                                                                                                                                                                                                                                                                                                                          |
| <i>real()</i>      | <b>(single)</b> - array to accept the <b>real</b> part of the error-term. One-dimensional for the number of data points.                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <i>imag()</i>      | <b>(single)</b> - array to accept the <b>imaginary</b> part of the error-term. One-dimensional for the number of data points.                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <b>Return Type</b> | Single                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |

**Default** Not Applicable

**Examples**

```
dim numpts as long
numpts = ActiveChannel.NumberOfPoints
ReDim r(numpts) ' real part
ReDim i(numpts) ' imaginary part
Dim CalSet as CalSet
set CalSet = pna.GetCalManager.GetCal SetByGUID(txtGUID)
Dim eData As ICalData2
Set eData = CalSet
eData.getErrorTermComplex 0, naET_LoadMatch, 1, 2, numpts,
r(0),i (0)
```

**C++ Syntax** HRESULT getErrorTermComplex(long setID, tagNAErrorTerm2 ETerm, long ReceivePort, long SourcePort, long\* pNumValues, float\* pReal, float\* plmag)

**Interface** ICalData2

## GetErrorTermComplexByString Method

---

**Description** Returns error term data from the Cal Set by specifying the string name.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

---

**Note:** This method exists on a non-default interface. If you cannot access this method, use [GetErrorTermByString](#)

---

**VB Syntax** *ICalData3*.GetErrorTermComplexByString *setNumber, errorTerm, numPoints, real(0), imag(0)*

**Variable** **(Type) - Description**

*ICalData3* An ICalData3 pointer to a [CalSet](#) (Object)

*setNumber* **(Long)** There can be more than one set of error terms in a Cal Set.

- *setNumber* **0** contains the original set of error terms for a Cal Set.
- *setNumbers* **> 0** contain Interpolated error terms. Interpolated error terms are generated when interpolation is required and destroyed when no longer used. [Learn about Interpolation](#).
- To determine the *setNumber* in use by a channel, see [GetCalSetUsageInfo](#)

*errorTerm* **(String)** The string name of error term in the Cal Set. An example string for port 3 directivity in a full 2 port cal might be "Directivity(3,3)".

For a list error term string names, use [Get ErrorTermList2](#)

*numPoints* **(Long)** An In/Out parameter.

On the way **in**, you specify the **max** number of values being requested.

On the way **out**, the PNA returns number of values actually returned.

*real* **(Single)** The real component of the complex data.

*imag* **(Single)** The imaginary component of the complex data.

**Return Type** Single

**Default** Not Applicable

**Examples** [See example](#)

**C++ Syntax** HRESULT GetErrorTermComplexByString(long etermSetID, BSTR bufferName, long\* lnumPoints, single\* real, single\* imag);

**Interface** ICalData3



**GetErrorTermList Method OBSOLETE**

**Description** **Note:** This command is replaced by `CalSet.getErrorTermList2`

Returns the list of Error Terms contained in this Cal Set for the CalType specified in the `OpenCal Set` method. Learn more about [reading and writing Cal Data using COM](#).

The list is a comma separated, textual representation of the error terms with the term name followed by the port path in parentheses:

Term (n, n),  
Term (m,n)

Before calling this method you must open the Cal Set with `OpenCal Set..` If the Cal set is not open, this method returns `E_NA_Cal Set_ACCESS_DENIED`.

Use `StringToNAErrorTerm2` to convert the list entrees to values that can be used with `GetErrorTerm` and `PutErrorTerm`.

---

**Note:** The port path designation (m n) indicates the ports that contribute to the error being compensated. Directivity, source match and reflection tracking are single port characteristics, designated in this list by (n n) where n equals the port being characterized.

Other terms characterize the interaction between ports. For example, the load match term is describing the match at port (m) while looking into port (n). Thus the notation (m n) indicates the two ports that contribute to the loadmatch error.

**VB Syntax** `CalSet.GetErrorTermList (SetID, count, strList)`

**Variable** **(Type) - Description**

`CalSet` **(object)** - A Cal Set object

`SetID` (long) - specifies the error term set to query. Use 0 for the master set.

`count` (long) - the number of error terms in the returned list

`strList` **(string)** - comma separated list of error terms found in Cal Set

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
dim count as Integer
dim list as string
OpenCalSet (naCalType_TwoPortSOLT 1, 2)
GetErrorTermList(0, count, list)
CloseCalSet()
```

Assuming the cal set contained the full set of error terms for this two-port Cal, the returned list would be:

```
"Directivity(1 1),SourceMatch(1 1),ReflectionTracking(1
1),TransmissionTracking(2 1),LoadMatch(2 1),Isolation(2
1),Directivity(2 2),SourceMatch(2 2),ReflectionTracking(2
2),TransmissionTracking(1 2),LoadMatch(1 2),Isolation(1 2)"
```

**C++ Syntax** `HRESULT GetErrorTermList (long ertermSetID, long* count, BSTR* strList);`



**Interface** ICalSet

## GetErrorTermList2 Method

---

**Description** Returns a list of error terms names found in the Cal Set containing the specified prefix.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

**VB Syntax** *list = CalSet.GetErrorTermList2(setNumber, calTypePrefix)*

**Variable** **(Type) - Description**

*list* **(Variant)** Variant containing a string array of error term names.

*CalSet* **(object)** - A [CalSet](#) object

*setNumber* **(Long)** There can be more than one set of error terms in a Cal Set.

- setNumber **0** contains the original set of error terms for a Cal Set.
- setNumbers **> 0** contain Interpolated error terms. Interpolated error terms are generated when interpolation is required and destroyed when no longer used. [Learn about Interpolation.](#)
- To determine the setNumber in use by a channel, see [GetCalSetUsageInfo](#)

*caltypePrefix* **(String)** The string used to identify Cal Set data as belonging to a specific Cal Type. This string is used as a filter so that only the error term names of interest are returned. If the prefix is empty, all terms are returned.

An example prefix for a two port cal on ports 2 and 3 might be: "Full 2 Port Cal (2,3)".

**Return Type** Variant

**Default** Not Applicable

**Examples** [See an Example](#)

**C++ Syntax** HRESULT GetErrorTermList2 (long SetNumber, BSTR caltypePrefix, VARIANT\* list)

**Interface** ICalSet2

## Get ExternalTestSetIO Method

---

**Description** This method returns the IExternalTestSetIO interface.

**VB Syntax** `app.GetExternalTestSetIO`

**Variable** **(Type) - Description**

`app` An Application **(object)**

**Return Type** IHWExternalTestSetIO

**Default** Not Applicable

**Example**

```
Dim app As AgilentPNA835x.Application
Dim ets As HWExternalTestSetIO
Set ets = app.GetExternalTestSetIO
```

**C++ Syntax** HRESULT GetExternalTestSetIO (IHWExternalTestSetIO  
\*\*ptestset);

**Interface** IApplication

Read-only

**GetFilterStatistics Method**

---

**Description** Returns all four Filter Statistics resulting from a [SearchFilterBandwidth](#). To retrieve individual filter statistics, use [meas.FilterCF](#), [meas.FilterBW](#), [meas.FilterLoss](#), [meas.FilterQ](#) properties.

**VB Syntax** *meas*.**GetFilterStatistics** *cf,bw,loss,q*

**Variable** **(Type) - Description**

*meas* A Measurement (**object**)

*cf,bw,loss,q* Dimensioned variables to store the returned values

**Return Type** **(double)** *cf*  
**(single)** *bw,loss,q*

**Default** Not Applicable

**Examples**

```
'Dimension variables
Dim cf as Double
Dim bw as Single
Dim loss as Single
Dim q as Single

meas.GetFilterStatistics cf,bw,loss,q
```

**C++ Syntax** HRESULT GetFilterStatistics(double\* centerFreq, float\* bw, float\* loss, float\* quality)

**Interface** IMeasurement

## GetGuid Method

---

**Description** Returns a string containing the GUID identifying this Cal Set. Each Cal Set is assigned a GUID (global unique ID). GUIDs are used to retrieve and select Cal Sets on the PNA. Learn more about [reading and writing Cal Data using COM](#).

**VB Syntax** `value = CalSet.GetGuid`

**Variable** **(Type) - Description**

*value* **(string)** - Variable to store the returned GUID

*CalSet* **(object)** - A Cal Set object

**Return Type** String

**Default** Not Applicable

**Examples** `guid = CalSet.GetGuid 'Read`

**C++ Syntax** HRESULT GetGUID( BSTR\* pGUIDString);

**Interface** ICalSet

## get\_InputVoltage Method

---

**Description** Reads the ADC input voltage from Analog IN (pin 14) of the AUX IO connector

**VB Syntax** `volts = AuxIO.get_InputVoltage`

**Variable** **(Type) - Description**

`volts` **(double)** - variable to store the return value

`AuxIO` **(object)** - A Hardware Auxiliary Input / Output object

**Return Type** Double

**Default** 0

**Examples**

```
Dim aux as HWAuxIO
Set aux = PNA.getAuxIO
volts = aux.get_InputVoltage 'read voltage on Analog In
(pin 14)
```

**C++ Syntax** HRESULT get\_InputVoltage ( double\* Voltage );

**Interface** HWAuxIO

## get\_Input1 Method

---

**Description** Reads a hardware latch that captures high to low transitions on Input1 of the Material Handler IO. Reading the latch causes it to reset and is ready for the next transition. The hardware latch is only capable of capturing one transition per query. Additional transitions are ignored until after the next query.

Momentarily driving Input1 high, then low, causes a transition to be detected and latched.

**VB Syntax** *inp1 = handlerIo.get\_Input1*

**Variable** **(Type) - Description**

*inp1* **(variant)** - A variable to store the return value

*handlerIo* **(object)** - A HandlerIO object

**Return Type** Variant -

**0** - a high to low transition occurred at Input1 since the last time it was queried.

**1** - no high to low transition occurred.

**Default** Not Applicable

**Examples** `input1 = handlerIo.get_Input1 'Read`

**C++ Syntax** HRESULT get\_Input1 (VARIANT\* Data );

**Interface** IHWMaterialHandlerIO

## Get MaterialHandlerIO Method

---

**Description** This method returns the MaterialHandlerIO interface.

**VB Syntax** `app.GetMaterialHandlerIO`

**Variable** (Type) - Description

`app` An Application (**object**)

**Return Type** IHWMaterialHandlerIO

**Default** Not Applicable

**Example**

```
Dim app As AgilentPNA835x.Application
Dim hand As HWMaterialHandlerIO
Set hand = app.GetMaterialHandlerIO
```

**C++ Syntax** HRESULT GetMaterialHandlerIO (IHWMaterialHandlerIO  
\*\*phand);

**Interface** IApplication



## GetNAComplex Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                 |
|--------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Retrieves complex data from the specified location. See also <a href="#">getComplex</a> and <a href="#">getData</a> Method.                                                                                                                                                                                                                                     |
| <b>VB Syntax</b>   | <i>measData</i> . <b>getNAComplex</b> <i>location</i> , <i>numPts</i> , <i>data</i>                                                                                                                                                                                                                                                                             |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                     |
| <i>measData</i>    | An IArrayTransfer interface which supports the Measurement object                                                                                                                                                                                                                                                                                               |
| <i>location</i>    | <b>(enum NADataStore)</b> - Where the data you want is residing. Choose from:<br>0 - naRawData<br>1 - naCorrectedData<br>2 - naMeasResult<br>3 - naRawMemory<br>4 - naMemoryResult<br>5 - naDivisor - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using <a href="#">DataToDivisor Method</a> . |
| <i>numPts</i>      | <b>(long integer)</b> - Number of data points requested<br>[out] - specifies number of data elements returned<br>[in] - specifies the data being requested or the capacity of the <i>dComplex</i> array                                                                                                                                                         |
| <i>data</i>        | <b>(NAComplex)</b> - A one-dimensional array of NaComplex to store the data.                                                                                                                                                                                                                                                                                    |
| <b>Return Type</b> | NAComplex                                                                                                                                                                                                                                                                                                                                                       |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                  |
| <b>Examples</b>    | <pre>Dim dComplex(201) AS NaComplex Dim measData As IArrayTransfer Dim pts as Long Set measData = app.ActiveMeasurement measData.getNAComplex naCorrectedData, pts, dComplex(0)</pre>                                                                                                                                                                           |
| <b>Notes</b>       | The data is stored as Real and Imaginary ( <b>Re</b> and <b>Im</b> ) members of the NaComplex user defined type. You can access each number individually by iterating through the array.<br><pre>For i = 0 to NumPts-1   dReal (i) = dcomplex (i).Re   dImag (i) = dcomplex (i).Im Next i</pre>                                                                 |
| <b>C++ Syntax</b>  | HRESULT getNAComplex(tagNADataStore DataStore, long* pNumValues, TsComplex* pComplex)                                                                                                                                                                                                                                                                           |
| <b>Interface</b>   | IArrayTransfer                                                                                                                                                                                                                                                                                                                                                  |

## GetNumberOfGroups Method

---

**Description** Returns the number of groups a channel has yet to acquire. To set the number of groups for a channel, use [Number Of Groups Method](#)

**VB Syntax** *value* = *chan*.**GetNumberOfGroups**

**Variable** (Type) - Description

*value* **(Long Integer)** - Number of groups

*chan* Channel **(object)**

**Return Type** **(Long Integer)**

**Default** Not Applicable

**Examples** `groups = chan.GetNumberOfGroups 'Read`

**C++ Syntax** HRESULT GetNumberOfGroups(long\* numberOfGroups);

**Interface** IChannel3

## get\_Output Method

---

**Description** Type 1 and Type2 configurations: Returns the last value written to the selected output pin.

Type3 configuration: Returns the current state of the selected output pin. If an Input1 trigger occurs, the state may not be the same value as was written.

All configurations: Data is written using put\_Output Method.

**VB Syntax** `data = handlerIo.get_Output (pin)`

**Variable (Type) - Description**

*data* **(variant)** - A variable to store the return value. The returned value will be one of the following:

**0** - TTL Low

**1** - TTL High

*handlerIo* **(object)** - A HandlerIO object

*pin* **(enum as NAMatHandlerOutput)** - output to read. Choose from:

**naOutput1 (0)**

**naOutput1User (1)**

**naOutput2 (2)**

**naOutput2User (3)**

[Learn about User Output](#)

**Return Type** Variant

**Default** Not Applicable

**Examples** `data = handlerIo.get_Output(naOutput1)`

**C++ Syntax** `HRESULT get_Output ( tagNAMatHandlerOutput Output, VARIANT* Data );`

**Interface** IHWMaterialHandlerIO

Read-only

**get\_OutputVoltage Method**

---

**Description** Reads voltages on the DAC/Analog Output 1 and Output 2 (pins 2 and 3 of the Aux I/O connector)

**VB Syntax** `volts = AuxIO.get_OutputVoltage (output)`

**Variable** **(Type) - Description**

`volts` **(double)** - variable to store the return value

`AuxIO` **(object)** - A Hardware Auxiliary Input / Output object

`output` **(variant)** Number of the output DAC to read voltage from. Choose from:

**1** - Output DAC 1 -(pin 3)

**2** - Output DAC 2 -(pin 2)

**Return Type** Double

**Default** Not Applicable

**Examples**

```
Dim aux as HWAuxIO
Set aux = PNA.getAuxIO
volts = aux.get_OutputVoltage(1) 'read voltage from Analog Out 1
(pin3)
```

**C++ Syntax** HRESULT get\_OutputVoltage( VARIANT Output, double\* Voltage );

**Interface** IHWAuxIO

**get OutputVoltageMode Method**

---

**Description** This command returns the mode of the selected "Analog Out" line on the Auxiliary IO connector. The modes give the user the option to have the requested voltage applied immediately or not until the sweep is done. To set the mode, use put OutputVoltageMode Method.

**VB Syntax** `mode = auxIo.get_OutputVoltageMode (output)`

**Variable (Type) - Description**

*mode* **(enum NAOutputVoltageMode)** - variable to store the returned mode.

**naWaitEOS** - While in this mode any voltage changes sent to the selected analog out will only get applied to the output between sweeps.

**naNoWait** - While in this mode any voltage changes sent to the selected analog out will occur right away without waiting until the end of a sweep, the voltage gets applied immediately.

*auxIo* **(object)** - A Hardware Auxiliary Input / Output object

*output* (double) Analog Output. Choose from **1** or **2**

**Return Type** enum as NAOutputVoltageMode

**Default** naWaitEOS

**Examples** `vOutMode = auxIo.get_OutputVoltageMode (1)`

**C++ Syntax** HRESULT get\_OutputVoltageMode(VARIANT Output, tagNAOutputVoltageMode\* pMode);

**Interface** IHWAuxIO

## GetPairedData Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
|--------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Retrieves pairs of data from the specified location.<br><hr/> <b>Note:</b> This method exists on a non-default interface. If you cannot access this method, use the <a href="#">Get Data Method</a> on IMeasurement. <hr/>                                                                                                                                                                                                                                |
| <b>VB Syntax</b>   | <i>measData</i> .getPairedData <i>location, format, numPts, d1, d2</i>                                                                                                                                                                                                                                                                                                                                                                                    |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <i>measData</i>    | An IArrayTransfer interface which supports the Measurement object                                                                                                                                                                                                                                                                                                                                                                                         |
| <i>location</i>    | <b>(enum NADataStore)</b> - Where the data you want is residing. Choose from:<br>0 - naRawData<br>1 - naCorrectedData<br>2 - naMeasResult<br>3 - naRawMemory<br>4 - naMemoryResult<br>5 - naDivisor - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using <a href="#">DataToDivisor Method</a> .                                                                                           |
| <i>format</i>      | <b>(enum NAPairedDataFormat)</b> - Format in which you would like the Paired data. Choose from:<br><br><ul style="list-style-type: none"> <li>• <b>naLinMagPhase</b> - Linear magnitude and phase</li> <li>• <b>naLogMagPhase</b> - Log magnitude and phase</li> <li>• <b>naReallmaginary</b> - Real and Imaginary</li> </ul> <hr/> <b>Note:</b> Selecting <b>naReallmaginary</b> format is the same as using the <a href="#">getComplex</a> method <hr/> |
| <i>numPts</i>      | <b>(long integer)</b> - Number of data points requested<br>[out] - specifies number of data elements returned<br>[in] - specifies the data being requested or the capacity of the <i>dPaired</i> array                                                                                                                                                                                                                                                    |
| <i>d1</i>          | <b>(single)</b> - Array to store the magnitude / real values                                                                                                                                                                                                                                                                                                                                                                                              |
| <i>d2</i>          | <b>(single)</b> - Array to store the phase / imaginary values                                                                                                                                                                                                                                                                                                                                                                                             |
| <b>Return Type</b> | Two Single arrays                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                            |

**Examples**

```
Dim logm() As Single
Dim phase() As Single
Public measData As IArrayTransfer
Set measData = app.ActiveMeasurement
Dim numpts As Long
numPoints = app.ActiveChannel.NumberOfPoints
ReDim logm(numPoints)
ReDim phase(numPoints)

measData.getPairedData naCorrectedData, naLogMagPhase,
numPoints, logm(0), phase(0)

Print values(0), values(1)
```

**C++ Syntax** HRESULT getPairedData(tagNADataStore DataStore, tagNAPairedDataFormat PairFormat, long\* pNumValues, float\* pReal, float\* plmag)

**Interface** IArrayTransfer

**get\_Port Method**

**Description** Returns the value from the specified "readable" port.

**VB Syntax** `data = handlerIo.get_Port (port)`

**Variable** **(Type) - Description**

`data` **(variant)** - A variable to store the return value. The following table shows what the returned data represents:

| Port | MSB.....LSB<br>8.....0 |
|------|------------------------|
| C    | C3...C0                |
| D    | D3...D0                |
| E    | D3...D0 + C3...C0      |

`handlerIo` **(object)** - A HandlerIO object

`port` **(enum as NAMatHandlerPort)** - port to get data from. Choose from:

**naPortC - (2)**

**naPortD - (3)**

**naPortE - (4)**

---

**Note:** Reading data from the Write-only ports (A,B,F,G,H) will return an error. Ports C and D must be put in Read mode before reading from C, D, or E using PortMode Property.

---

**Return Type** Variant

**Default** 0

**Examples** `data = handlerIo.get_Port (naPortC)`

**C++ Syntax** `HRESULT get_Port ( tagNAMatHandlerPort Port, VARIANT* Data );`

**Interface** IHWMaterialHandlerIO



## get\_PortCData Method

---

**Description** Reads a 4-bit value from Port C of the Aux I/O connector (pins 22-25) and the Material Handler IO (pins 21-24 Anritsu) - (pins 22-25 Avantest).

**Note:** These lines are connected to both the Handler IO and Aux IO in the PNA.

**VB Syntax** `value = AuxIO.get_PortCData`

**Variable** **(Type) - Description**

`value` **(variant)** - Variable to store the returned data

`AuxIO` **(object)** - A Hardware Auxiliary Input / Output object

**Return Type** Integer

**Default** None

**Examples** `value = auxIo.get_PortCData 'Reading a value of 15 when in Positive Logic indicates Port C lines C0, C1, C2, C3 are High. If in Negative Logic they are Low.`

**C++ Syntax** `HRESULT get_PortCData( VARIANT* Data );`

**Interface** IHWAuxIO

## GetReferenceMarker Method

---

**Description** Returns a handle to the reference marker.

**VB Syntax** *meas*.GetReferenceMarker

**Variable** (Type) - Description

*meas* A Measurement (**object**)

**Return Type** Object

**Default** Not Applicable

**Examples** `meas.GetReferenceMarker`

**C++ Syntax** HRESULT GetReferenceMarker(IMarker\*\*  
refMarker)

**Interface** IMeasurement

**GetRequiredEtermNames**

---

**Description** Returns an array of strings specifying the error terms required by the caltype's correction algorithm in order to correct the specified parameter.

This function interrogates a specific caltype ( caltypeGUID) for the list of error terms it would need in order to correct the specified parameter. All the standard S Parameter calibration types embed port specifiers in the error term name. The specific port information is gleaned from the passed parameter. For example, to query the error term requirements specific to a two port cal on ports 1 and 3, issue this with a parameter of S13 or S31. The buffer names returned will be formatted in this way:

Full 1 Port SOLT(1,3):TransmissionTracking(3,1)

**VB Syntax** **EtermNames = GetRequiredEtermNames**(CalTypeGUID As String, Parameter As String)

**Variable** **(Type) - Description**

*caltypeGUID*: [in] the GUID of the desired calibration type

*parameter* [in] string specifying the parameter to be corrected

EtermNames [out] array of strings containing the error term names.

---

**Note:** In C++ Allocated by server. Must be freed by caller using SysFreeString.

---

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** enames = GetRequiredEtermNames(ctGUID, Parm)

**C++ Syntax** HRESULT GetRequiredEtermNames( BSTR caltypeGUID, BSTR parameter, VARIANT\* EtermNames )

**Interface** ICalManager2

## GetScalar Method

---

**Description** Retrieves scalar data from the specified locations.

**Note:** This method exists on a non-default interface. If you cannot access this method, use the [Get Data Method](#) on IMeasurement.

**Note:** You can **NOT** use this command to get complex data.

**VB Syntax** *measData.getScalar location, format, numPts, data*

**Variable** **(Type) - Description**

*measData* An IArrayTransfer interface which supports the Measurement object

*location* **(enum NADataStore)** - Where the data you want is residing. Choose from:

0 - naRawData

1 - naCorrectedData

2 - naMeasResult

3 - naRawMemory

4 - naMemoryResult

5 - naDivisor - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using [DataToDivisor Method](#).

*format* **(enum DataFormat)** - Scalar format in which you would like the data. Choose from:

- naDataFormat\_Delay
- naDataFormat\_Imaginary
- naDataFormat\_LinMag
- naDataFormat\_LogMag
- naDataFormat\_Phase
- naDataFormat\_Real
- naDataFormat\_SWR

*numPts* **(long integer)** - Number of data points requested  
 [out] - specifies number of data elements returned  
 [in] - specifies the data being requested or the capacity of the *dScalar* array

*data* **(single)** - Array to store the scalar data.

**Return Type** Single

**Default** Not Applicable

**Examples**

```
Dim dScalar() As Single
Dim measData As IArrayTransfer
Set measData = app.ActiveMeasurement
Dim numpts as Long
numpts = app.ActiveChannel.NumberOfPoints
ReDim dScalar(numPoints)

measData.getScalar naCorrectedData, naDataFormat_LogMag, numpts,
dScalar(0)
Print dScalar(0), dScalar(1)
```

**C++ Syntax** HRESULT getScalar(tagNADataStore DataStore, tagDataFormat DataFormat, long\* pNumValues, float\* pVals)

**Interface** IArrayTransfer

Read-only

## GetShortcut Method

---

**Description** Returns the Title, Path, and optional argument strings, of the specified Macro (shortcut). Use this method to list the titles and paths of macros in the analyzer.

**VB Syntax** *app*.GetShortcut *index*, *title*, *path*, *arguments*

**Variable** **(Type) - Description**

*app* An Application (**object**)

*index* (**long**) - Number of the macro. Use a number between **1** and **12**.

*title* (**string**) - **Title** of the specified macro. (Appears in the softkey label)

*path* (**string**) - **Pathname** of the specified macro.

*arguments* (**string**) - Arguments for the specified macro

**Return Type** String

**Default** Not Applicable

**Example**

```
Dim t As String
Dim p As String
Dim arg As String
Dim i As Integer
For i = 1 to 12
 app.GetShortcut i,t,p,arg
 Print t,p
Next
```

**C++ Syntax** HRESULT GetShortcut(long Number, BSTR\* title, BSTR\* pathname, BSTR\* arguments)

**Interface** IApplication

**Remarks** Shortcuts can also be defined and accessed using the macro key on the front panel. However, the benefit of this feature is primarily for the interactive user

**GetSnPData Method**

---

**Description** Reads SnP data from the selected measurement. [Learn more about SnP that is returned from the PNA.](#)

**VB Syntax** `data = meas.GetSnPData type`

**Variable (Type) - Description**

`data` Variant array to store the data.

`meas` A Measurement (**object**)

`type` (**string**) - Type of SnP data to return. If unspecified, <n> is set to 2. Choose from:

"S1P" returns data for the active measurement.

"S2P" returns data for the current 2-port measurement (4 S-parameters).

"S3P" returns data for the current 3 port measurement (9 S-parameters). Valid only on instruments with more than 2 ports.

SnP data can be output using several data formatting options. See [SnPFormat Property](#)

**Return Type** Variant array - automatically dimensioned to the size of the data

**Default** Not Applicable

**Examples**

```
Dim pna As AgilentPNA835x.Application
Dim meas As AgilentPNA835x.IMeasurement3
Dim snp
Set pna = CreateObject("AgilentPnA835x.application")
Set meas = pna.ActiveMeasurement
snp = meas.GetSnPData("s2p")

Dim param
Dim point

' snp returns a 3 dimensional array
' dimension 1 is the parameter, s11, s21, s12, s22
' snp(param,point,pair)
'-----
For param = LBound(snp, 1) To UBound(snp, 1)
 Debug.Print "Parameter: " & (param + 1)
 For point = LBound(snp, 2) To UBound(snp, 2)
 Debug.Print " Point: " & (point + 1)
 Debug.Print " Real", snp(param, point, 0) ' real element
 Debug.Print " Imag", snp(param, point, 1) 'imaginary
 element
 Next
Next
```

**C++ Syntax** HRESULT GetSnPData( BSTR snptype, VARIANT \* response)

**Interface** IMeasurement3





Read-only

**getSourcePowerCalDataEx Method**

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p><b>Note:</b> This method replaces <a href="#">getSourcePowerCalData Method</a></p> <p>Retrieves (as variant data type) source power calibration data, if it exists, from the channel.</p> <p>If the channel is sweeping the source backwards, then the first data point is the highest frequency value; the last data point is the lowest. Use the <a href="#">Get X-Axis Values</a> command to return the X-axis values in the displayed order.</p> <p><b>Note:</b> This method returns a variant which is less efficient than methods available on the <a href="#">ISourcePowerCalData</a> interface</p> |
| <b>VB Syntax</b>   | <code>data = chan.getSourcePowerCalData (buffer, sourcePort)</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |
|                    | <code>data</code> <b>(variant)</b> – Array to store the data.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|                    | <code>chan</code> <b>(object)</b> – A <a href="#">Channel</a> object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
|                    | <code>buffer</code> <b>(enum NASourcePowerCalBuffer)</b> - The requested source power cal data buffer.<br><b>0 - naCorrectionValues</b> This is the only buffer currently available                                                                                                                                                                                                                                                                                                                                                                                                                           |
|                    | <code>sourcePort</code> <b>(long integer)</b> – The source port for which calibration data is being requested.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Return Type</b> | Variant array – automatically dimensioned to the size of the data.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Examples</b>    | <pre>Dim varData As Variant Const port1 As Long = 1 varData = chan.getSourcePowerCalDataEx (naCorrectionValues, port1) 'Print the data For i = 0 to chan.NumberOfPoints - 1 Print varData(i) Next i</pre>                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>C++ Syntax</b>  | HRESULT getSourcePowerCalDataEx(tagNASourcePowerCalBuffer bufSelect, long sourcePort, VARIANT *pData);                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| <b>Interface</b>   | IChannel4                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |

**getSourcePowerCalDataScalarEx Method**

**Description** Note: This method replaces getSourcePowerCalDataScalar Method

Retrieves (as scalar values) source power calibration data, if it exists, from this channel. If the channel is sweeping the source backwards, then the first data point is the highest frequency value; the last data point is the lowest. Use the Get X-Axis Values2 command to return the X-axis values in the displayed order.

Note: This method exists on a non-default interface. If you cannot access this method, use the getSourcePowerCalDataEx Method on IChannel4.

**VB Syntax** *chanData.getSourcePowerCalDataScalar* *buffer, sourcePort, numValues, data*

**Variable** (Type) - Description

*chanData* **(interface)** – An ISourcePowerCalData2 interface on the Channel object.

*buffer* **(enum NASourcePowerCalBuffer)** - The requested source power cal data buffer.  
**0 - naCorrectionValues** Currently this is the only buffer available.

*sourcePort* **(long integer)** – The source port for which calibration data is being requested.

*numValues* **(long integer)** – Number of data values.  
 [out] – specifies number of data values returned.  
 [in] – specifies number of values being requested (this must not be larger than the capacity of the data array).

*data* **(single)** – Array to store the data.

**Return Type** Single

**Default** Not Applicable

**Examples**

```
Dim numValues As Long
Dim scalarCalValues() As Single
Dim chanData As ISourcePowerCalData2
Const port1 As Long = 1
numValues = app.ActiveChannel.NumberOfPoints
ReDim scalarCalValues(numValues)
Set chanData = app.ActiveChannel

chanData.getSourcePowerCalDataScalarEx naCorrectionValues,
port1, numValues, scalarCalValues(0)

'Print the data
For i = 0 to numValues - 1
Print scalarCalValues(i)
Next I
```

**C++ Syntax** HRESULT getSourcePowerCalDataScalarEx(tagNASourcePowerCalBuffer bufSelect, long sourcePort, long \*pNumValues, float \*pData);

**Interface** ISourcePowerCalData2

**GetStandard Method OBSOLETE**

---

**Description** This command has been replaced with [Get StandardByString](#)

Returns standard acquisition data from the Cal Set. The returned data is complex pairs.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

**VB Syntax** `data = CalSet.getStandard (standard, rcv, src)`

**Variable (Type) - Description**

*data* **(Variant)** Two-dimensional safe array to store the returned data. Memory for the returned Variant is allocated by the PNA and must be released by client.

**Note:** See also [getStandardComplex](#) on the ICalData2 interface to avoid using the variant data type.

*CalSet* **A Cal Set (object)**

*standard* **(enum NACalClass)** Standard data to be read. Choose from:

- 1 - naClassA
- 2 - naClassB
- 3 - naClassC
- 4 - naClassD
- 5 - naClassE
- 6 - naReferenceRatioLine
- 7 - naReferenceRatioThru

**SOLT Standards**

- 1 - naSOLT\_Open
- 2 - naSOLT\_Short
- 3 - naSOLT\_Load
- 4 - naSOLT\_Thru
- 5 - naSOLT\_Isolation

**TRL Standards**

- 1 - naTRL\_Reflection
- 2 - naTRL\_Line\_Reflection
- 3 - naTRL\_Line\_Tracking
- 4 - naTRL\_Thru
- 5 - naTRL\_Isolation

*rcv* **(long)** - Receiver Port

*src* **(long)** - Source Port

**Return Type** **(variant)**

**Default** Not Applicable

**Examples**

```
Dim varStd As Variant
Dim varStd2 As Variant

Cal Set.OpenCalSet(naCalType_TwoPortSOLT, 1, 2)
varStd = CalSet.getStandard(naSOLT_Thru,2,1)
varStd2 = Cal Set.getStandard(naSOLT_Thru,1,2)
Cal Set.CloseCalSet()
```

**C++ Syntax** HRESULT getStandard(tagNACalClass stdclass, long ReceivePort, long SourcePort, VARIANT\* pData)

**Interface** ICalSet

## GetStandardByString Method

---

**Description** Returns standard acquisition data from the Cal Set. The returned data is complex pairs.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

**VB Syntax** `data = calSet.GetStandardByString(stdName)`

**Variable** **(Type) - Description**

*data* **(Variant)** Two-dimensional safe array to store the returned data. Memory for the returned Variant is allocated by the PNA and must be released by client.

---

**Note:** See also [Get StandardComplexByString](#) on the ICalData2 interface to avoid using the variant data type.

---

*calSet* A [CalSet](#) **(Object)**

*stdName* **(String)** The string used to identify a particular standard in the Cal Set. An example string requesting the data for the Load standard in a full 2 port cal might be "S11C(3,3)".

**Return Type** Variant

**Default** Not Applicable

**Examples** See an [example](#)

**C++ Syntax** HRESULT GetStandardByString( BSTR bufferName, VARIANT\* pdata)

**Interface** ICalSet2

**GetStandardComplex Method OBSOLETE**

---

**Description** This command is replaced with GetStandardComplexByString

Returns standard acquisition data from the Cal Set. The returned data is complex pairs.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

---

**Note:** This method exists on a non-default interface. If you cannot access this method, use the [GetStandard](#) Method on [ICal Set](#)

---

**VB Syntax** *ICalData2*.**getStandardComplex** *class, rcv, src, numPts, real(), imag()*

**Variable** **(Type) - Description**

*ICalData2* An [ICalData2](#) pointer to the Cal Set object

*class* **(enum NACalClass)** Standard data to be read. Choose from:

- 1 - naClassA
- 2 - naClassB
- 3 - naClassC
- 4 - naClassD
- 5 - naClassE
- 6 - naReferenceRatioLine
- 7 - naReferenceRatioThru

**SOLT Standards**

- 1 - naSOLT\_Open
- 2 - naSOLT\_Short
- 3 - naSOLT\_Load
- 4 - naSOLT\_Thru
- 5 - naSOLT\_Isolation

**TRL Standards**

- 1 - naTRL\_Reflection
- 2 - naTRL\_Line\_Reflection
- 3 - naTRL\_Line\_Tracking
- 4 - naTRL\_Thru
- 5 - naTRL\_Isolation

*rcv* **(long)** - Receiver Port

*src* **(long)** - Source Port

*numPts* **(Long)** An In/Out parameter.

On the way **in**, you specify the **max** number of values being requested.

On the way **out**, the PNA returns number of values actually returned.

*real()* **(single)** - array to accept the real part of the calibration data. One-dimensional for the number of data points.

*imag()* **(single)** - array to accept the imaginary part of the calibration data. One-dimensional for the number of data points.

**Return Type** **(single)**

**Default** Not Applicable

**Examples**

```
Dim numpts as long
numpts = ActiveChannel.NumberOfPoints
ReDim r(numpts) ' real part
ReDim i(numpts) ' imaginary part
Dim Cal Set as Cal Set
set Cal Set = pna.GetCalManager.GetCal SetByGUID(txtGUID)
Dim sData As ICalData2
Set sData = Cal Set
sdata.getStandardComplex naSOLT_Open, 1, 1, numpts, r(0), i(0)
```

**C++ Syntax** HRESULT getStandardComplex(tagNACalClass stdclass, long ReceivePort, long SourcePort, long\* pNumValues, float\* pReal, float\* plmag)

**Interface** ICalData2



## GetStandardComplexByString Method

---

**Description** Returns standard acquisition data from the Cal Set.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

**VB Syntax** *ICalData3*.**GetStandardComplexByString** *stdName, InumPoints, real(0), imag(0)*

**Variable (Type) - Description**

*ICalData3* An [ICalData3](#) pointer to a [CalSet](#) (**Object**)

*stdName* (**String**) The string used to identify a particular standard in the Cal Set. An example string requesting the data for the Load standard in a full 2 port cal might be "S11C(3,3)".

*InumPoints* (**Long**) An In/Out parameter.

On the way **in**, you specify the **max** number of values being requested.

On the way **out**, the PNA returns number of values actually returned.

*real* (**Single**) The real component of the complex data.

*imag* (**Single**) The imaginary component of the complex data.

**Return Value** Single

**Default** Not Applicable

**Examples** [See example](#)

**C++ Syntax** HRESULT GetStandardComplexByString( BSTR bufferName, long\* InumPoints, float\* real, float\* imag);

**Interface** ICalData3

**GetStandardsList Method OBSOLETE**

---

**Description** Note: This command is replaced by [CalSet.getStandardList2](#).

Returns the list of Standards contained in this Cal Set for the CalType specified in the [OpenCal Set](#) method. Learn more about [reading and writing Cal Data using COM](#).

The list is a comma separated, textual representation of the error terms with the term name followed by the port path in parentheses.

Standard (n, n),  
Standard (m, n)

Before calling this method you must open the Cal Set with [OpenCal Set](#). If the Cal Set is not open, this method returns E\_NA\_Cal Set\_ACCESS\_DENIED.

Use [StringToNACalClass](#) to convert the list entrees to values that can be used with [GetStandard](#) and [PutStandard](#).

**Note:** The port path designation (m n) indicates the receive and source ports for the measurement. Shorts, opens and loads are single port devices, designated in this list by (n n) where n equals the port to which the device is connected. These devices are all characterized by reflection measurements.

The dual port thru device is characterized by both transmission and reflection measurements in order to compensate for load match and tracking terms.

The notation (n n) indicates the reflection measurement for this device.

The notation (m n) indicates the transmission measurement, where the source and receive ports are different.

**VB Syntax** *CalSet*.**GetStandardsList** (*count*, *list*)

**Variable** **(Type) - Description**

*CalSet* **(object)** - A Cal Set object

*count* **(long [out])** - indicates the number of items returned in the list

*list* **(string)** - Variable to store the returned Comma separated list of items.

**Return Type** String

**Default** Not Applicable

**Examples**

```
dim count as Integer
dim list as string
OpenCalSet (naCalType_TwoPortSOLT, 1, 2)
GetStandardsList(count, list)
CloseCalSet()
```

Assuming the Cal Set contained the full set of standards for this two port cal, the returned list would be:

```
"Open(1 1),
Short(1 1),
Load(1 1),
Thru(1 1),
Isolation(2 1),
Open(2 2),
Short(2 2),
Load(2 2),
Thru(2 2),
Isolation(1 2)
Thru(2 1),
Thru(1 2)"
```

**C++ Syntax** HRESULT GetStandardsList( long\* count, BSTR\* list);

**Interface** ICalSet

## GetStandardList2 Method

---

**Description** Returns a list of standards contained by this Cal Set for the specified Cal Type.

**VB Syntax** *list* = *calset*.**GetStandardList2**(*calType*)

**Variable** **(Type) - Description**

*calset* **(object)** - A [CalSet](#) object

*list* **(Variant)** Variant containing a string array of standards for the specified calType.

*calType* **(String)** The string used to identify Cal Set data as belonging to a specific Cal Type. This string is used as a filter so that only the standard names of interest are returned. If the prefix is empty, all names are returned.

An example prefix for a two port cal on ports 2 and 3 might be: "Full 2 Port Cal (2,3)".

**Return Type** Variant

**Default** Not Applicable

**Examples** [See an example](#)

**C++ Syntax** HRESULT GetStandardList2 (BSTR caltype, VARIANT\* list)

**Interface** ICalSet2

## GetStandardsForClass Method

---

**Description** Get the calibration standard numbers for a specified calibration class. To set the calibration number use [SetStandardsForClass Method](#)

**VB Syntax** *calkit*.**GetStandardsForClass** (*calclassorder*, *std1*, *std2*, *std3*, *std4*, *std5*, *std6*, *std7*)

**Variable** **(Type) - Description**

*calKit* A CalKit (**object**)

*calclassorder* **(enum NACalClassOrder)** Choose from:

- 0 - naRefl\_1\_S11
- 1 - naRefl\_2\_S11
- 2 - naRefl\_3\_S11
- 3 - naTran\_1\_S21
- 4 - naRefl\_1\_S22
- 5 - naRefl\_2\_S22
- 6 - naRefl\_3\_S22
- 7 - naTran\_1\_S12
- 8 - naRefl\_1\_S33
- 9 - naRefl\_2\_S33
- 10 - naRefl\_3\_S33
- 11 - naTran\_1\_S32
- 12 - naTran\_1\_S23
- 13 - naTran\_1\_S31
- 14 - naTran\_1\_S13
- 15 - naTRL\_T
- 16 - naTRL\_R
- 17 - naTRL\_L

*std1...std7* **(long)** Calibration Standard Number. Nominal values from 1 through 30. 0 indicates that a standard number has not been selected.

**Return Type** Not applicable

**Default** Not applicable

**Examples** `calkit.GetStandardsForClass naRef1_3_S11, std1, std2, std3, std4, std5, std6, std7`

**C++ Syntax** HRESULT GetStandardsForClass(NACalClassOrder calclassorder, long std1, long std2, long std3, long std4, long std5, long std6, long std7)

**Interface** ICalkit

Read-only

## GetStepDescription Method

---

**Description** Returns the description of the specified step in the calibration process.

**VB Syntax** *value* = *obj*.**GetStepDescription** (*n*)

**Variable** **(Type) - Description**

*value* (string) - Variable to store the returned number of steps.

*obj* Any of the following:

GuidedCalibration (object)

SMCType (object)

VMCType (object)

*n* (Long) Step in the calibration process.

Use GenerateSteps to determine the total number of steps.

**Return Type** String

**Default** Not Applicable

**Examples** `value = SMC.GetStepDescription(5)`

**C++ Syntax** HRESULT get\_GetStepDescription(long step, BSTR\* str);

**Interface** IGuidedCalibration

SMCType

VMCType

## GetTestResult Method

---

**Description** Returns the result of limit line testing. There are three ways to use this command:

- If neither optional parameter is specified, limit results for ALL data is returned.
- If one parameter is specified (*start*), the limit result for that data point is returned.
- If both parameters are specified, limit results are returned beginning with *start*, and ending with (*start+size*)-1

**VB Syntax** `testRes = limts.GetTestResult [start,size]`

**Variable** **(Type) - Description**

*testRes* **(enum NALimitTestResult)** - A dimensioned variable to store test results. If a limit line is not tested, a PASS is returned.

0 - naLimitTestResult\_None

1 - naLimitTestResult\_Fail

2 - naLimitTestResult\_Pass

*limts* A LimitTest **(object)**

*start* **(long)** - Optional argument. A start data point number to return limit test results.

*size* **(long)** - Optional argument. Number of data points from *start* to return limit test results.

**Return Type** Long Integer

**Default** Not Applicable

**Examples**

```
Dim testRes As NALimitTestResult
testRes = limts.GetTestResult
Select Case testRes

Case 1
Print "Fails"

Case 2
Print "Pass"

End Select
```

**C++ Syntax** HRESULT GetTestResult(long IStart, long ISize, tagNALimitTestResult \*pVal)

**Interface** ILimitTest



Read-only

## GetTraceStatistics Method

---

**Description** Returns all four Trace Statistics. To retrieve individual Trace statistics, use [Mean](#), [PeakToPeak](#), [StandardDeviation](#) properties. Use [ShowStatistics](#) to display the statistics of the screen.

**VB Syntax** *meas*.GetTraceStatistics *pp,mean,stdev*

**Variable** **(Type) - Description**

*meas* A Measurement (**object**)

*pp,mean,stdev* (**double**) - Dimensioned variables to store the returned values

**Return Type** Double

**Default** Not Applicable

**Examples**

```
'Dimension variables
Dim pp As Double
Dim mean As Double
Dim stdv As Double
meas.GetTraceStatistics pp, mean, stdv
```

**C++ Syntax** HRESULT GetTraceStatistics(double\* pp, double\* mean, double\* stdDeviation)

**Interface** IMeasurement

## GetXAxisValues2 Method

---

**Description** Returns the channel's X-axis values into a dimensioned Typed array. GetXAxisValues2 is a convenient method for determining the frequency of each point when the points are not linearly spaced - as in segment sweep.

---

**Note:** This method will fail if called using a scripting client such as VBScript or Agilent Vee, (see remarks)

---

**Note:** In Segment Sweep, `chan.NumberofPoints` will return the total number of data points for the combined segments.

---

**VB Syntax** `chan.GetXAxisValues2 numPts,data`

**Variable** **(Type) - Description**

`chan` **(object)** - A Channel object

`numPts` **(long integer)** - Number of data points in the channel

`data` **(double)** Single dimensioned array of data matching the number of points in the channel.

**Return Type** double

**Default** Not applicable

**Examples**

```
Dim App As Application
Set App = New Application
Dim numPoints As Long
Dim values() As Double
numPoints = App.ActiveChannel.NumberOfPoints
ReDim values(numPoints)
App.ActiveChannel.GetXAxisValues2 numPoints, values(0)
Print values(0), values(1)
```

**C++ Syntax** HRESULT GetXAxisValues2(long\* pNumValues, double\* stimulus)

**Interface** IChannel

### Remarks:

This method will fail if called using a scripting client such as VBScript or Agilent Vee. Use the [GetXAxisValues](#) method as a replacement for these COM environments.

This method also cannot be called using late-bound typing in Visual Basic. For instance, if, in the example above, the first line were replaced with "Dim App as Object", then this method would fail.

Read-only

## GetXAxisValues Method

---

**Description** Returns the stimulus values for the measurement. To understand how this property is useful, see [IMeasurement2 Interface](#).

**VB Syntax** *data* = *meas*.GetXAxisValues

**Variable** (Type) - Description

*data* **(Variant)** Array to store the data.

*meas* A Measurement **(object)**

**Return Type** Variant

**Default** Not Applicable

**Examples**

```
Dim varData As Variant
Dim i As Integer
varData = meas.GetXAxisValues
'Print Data
For i = 0 To meas.NumberOfPoints - 1
Print varData(i)
Next i
```

**C++ Syntax** HRESULT GetXAxisValues(VARIANT\* xData);

**Interface** IMeasurement2

## GetXAxisValues Method

---

**Description** Returns the channel's X-axis values. GetXAxisValues is a convenient method for determining the frequency of each point when the points are not linearly spaced - as in segment sweep.

---

**Note:** This method returns a variant which is less efficient than [GetXAxisValues2](#).

---

**Note:** In Segment Sweep, chan.NumberOfPoints will return the total number of data points for the combined segments.

---

**VB Syntax** `data = chan.GetXAxisValues`

**Variable** **(Type) - Description**

`data` Variant array to store the data.

`chan` A Channel (**object**)

**Return Type** Variant

**Default** Not Applicable

**Examples**

```
Dim varData As Variant
Dim i As Integer
varData = chan.GetXAxisValues
'Print Data
For i = 0 To chan.NumberOfPoints - 1
 Print varData(i)
Next i
```

**C++ Syntax** HRESULT GetXAxisValues (VARIANT\* xData)

**Interface** IChannel

## HasCalType Method

---

**Description** Verifies that the Cal Set object contains the error terms required to perform the specified correction (CalType) to an appropriate measurement.

The argument list includes specifiers for up to 3 ports. The number of arguments required depends on the CalType specified. The value for each port is set to 0 if not specified.

**VB Syntax** `check = CalSet.HasCalType (calType, p1, p2, p3)`

**Variable** (Type) - Description

*check* **(boolean)** - variable to store the returned value

**TRUE (1)** - Cal Set has all of the error terms necessary to apply the specified correction CalType.

**FALSE(0)** - Cal Set DOES NOT have all of the error terms necessary to apply the specified CalType.

*CalSet* **(object)** - A Cal Set object

*calType* (enum as naCalType) - type of correction to be applied. Choose from:

| <b>Caltype</b>                               | <b>p arguments required</b>       |
|----------------------------------------------|-----------------------------------|
| <b>0</b> - naCalType_Response_Open           | p1                                |
| <b>1</b> - naCalType_Response_Short          | p1                                |
| <b>2</b> - *naCalType_Response_Thru          | p1 (rcv), p2 (src)                |
| <b>3</b> - *naCalType_Response_Thru_And_Isol | p1 (rcv), p2 (src)                |
| <b>4</b> - naCalType_OnePort                 | p1                                |
| <b>5</b> - naCalType_TwoPort_SOLT            | p1, p2                            |
| <b>6</b> - naCalType_TwoPort_TRL             | p1, p2                            |
| <b>7</b> - naCalType_None                    | N/A                               |
| <b>8</b> - naCalType_ThreePort_SOLT          | p1, p2, p3                        |
| <b>9</b> - Custom                            | N/A                               |
| <b>10</b> - naCalType_FourPort_SOLT          | p1, p2, p3<br>(port 4 is assumed) |

\* order of port arguments is significant for these CalTypes

*p1* **(long)** - required. This argument must be specified.

This specifies either:

- the one significant port for an open/short response cal or a 1 port cal.
- or one of the ports involved in a 2, 3, or 4 port cal
- or the **receive** port for a thru response / thru-isolation cal.

*p2* **(long)** - required for any CalType involving more than one port

This specifies either:

- one of the ports involved in a 2, 3, or 4 port cal (order independent)
- or the **source** port for a thru response / thru-isolation cal

*p3* **(long)** - required for 3 and 4-port cal

This specifies one of the ports involved in a 3 or 4 port cal (order independent)

**Return Type** **VARIANT\_BOOL**

**Default** Not Applicable

**Examples** `value = CalSet.HasCalType(naCalType_TwoPort_TRL, 1, 2)`

**C++ Syntax** HRESULT HasCalType( tagNACalType, long port1, long port2, long port3, BOOL \*pVal);

**Interface** ICalSet

## Hold Method

---

**Description** Puts the Channel in Hold - not sweeping.

**VB Syntax** `chan.Hold [sync]`

**Variable** (Type) - Description

`chan` A Channel (**object**)

`[sync]` (**boolean**) - Optional argument. A variable set to either True or False.

**True** - program control waits until the channel is in the Hold state.

**False** - program control continues immediately. You are not guaranteed the channel is in Hold yet.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
wate = True
chan.Hold wate
```

**C++ Syntax** HRESULT Hold(VARIANT\_BOOL bWait)

**Interface** IChannel

## Hold (channels) Method

---

**Description** Places all channels in hold mode. To place a single channel in hold mode, use [channel.Hold](#) Method.

**VB Syntax** *chans.Hold*

**Variable** **(Type) - Description**

*chans* A [Channel collection](#) (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `chans.Hold`

**C++ Syntax** HRESULT Hold();

**Interface** IChannels2



Write only

## Initialize Method

---

**Description** Begins a calibration.

**Note:** *chan* must be the active channel.

---

**VB Syntax** *obj.Initialize (chan, useCalReg)*

**Variable** **(Type) - Description**

*obj* Any of the following:

GuidedCalibration (object)

SMCType (object)

VMCType (object)

*chan* (Long) Channel number to calibrate.

*useCalReg* (boolean)

**True** or **1** - Cal will be stored in Cal Register ONLY

**False** or **0** - Cal will be stored in Cal Register AND User Cal Set. The active channel must be pointing to a User Cal Set.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `smc.Initialize(2,1)`

**C++ Syntax** HRESULT put\_Initialize(long channelnumber, VARIANT\_BOOL bNewCalSet);

**Interface** IGuidedCalibration

SMCType

VMCType

**Item Method**

---

**Description** Returns an object from the collection of objects.

**Note:** The order of objects within a collection cannot be assumed.

**VB Syntax** *Object* [.Item](*n*)

**Variable** **(Type) - Description**

*Object* Any of the following **(objects)**:  
 CalFactorSegments collection  
 Cal Sets collection  
 Channels collection  
 LimitTest collection  
 Measurements collection  
 NaWindows collection  
 PowerLossSegments collection  
 PowerSensors collection  
 Segments collection  
 Traces collection

**.Item** Optional - Item is the default property of a collections object and therefore can be called implicitly. For example, the following two commands are equivalent:

```
Channels.Item(3).Averaging = 1
Channels(3).Averaging = 1
```

*n* **(variant)** - number of the item in the collection.

**Note:** The Measurements and Traces collections allow you to specify the name of the measurement as a string. For example:

```
measCollection("CH_S11_1").InterpolateMarkers
```

**Return Type** **(Object)**

**Default** Not Applicable

**Examples**

```
For i = 1 to Traces.Count - 1
 Traces.Item(i).YScale = .5dB
Next i
```

**C++ Syntax** HRESULT Item(VARIANT index, <interface>\*\* pItem)

**Interfaces** ICalFactorSegments  
 ICal Sets  
 IChannels  
 ILimitTest  
 IMeasurements  
 INaWindows  
 IPowerLossSegments  
 IPowerSensors  
 ISegments  
 ITraces



**LaunchCalWizard Method**

---

**Description** Launches the Cal Wizard on the PNA and does not return until the Cal Wizard is dismissed.

---

**Note:** The Cal Wizard operates on the active measurement. Therefore, activate the measurement to be calibrated before launching the Cal Wizard.

---

**VB Syntax** `success = app.LaunchCalWizard (newCS)`

**Variable (Type) - Description**

`success` **(boolean)** - variable to store the returned value  
**True** - The Cal was completed  
**False** - The Cal was canceled without completing the calibration.

`app` An Application **(object)**

`newCS` **(boolean)**  
**True** - Cal will be performed on a new Cal Set.  
**False** - Cal will be performed using the existing Cal Set assigned to the channel. If no Cal Set is found, a new Cal Set will be created.

**Return Type** Boolean

**Default** Not Applicable

**Example**

```
dim bSuccess as boolean
dim bNewCalset as boolean
bNewCalSet = false
bSuccess = app.LaunchCalWizard(bNewCalSet)
```

**C++ Syntax** HRESULT LaunchCalWizard(VARIANT\_BOOL bCalsuccess)

**Interface** IApplication

## LaunchPowerMeterSettingsDialog Method

---

**Description** Launches the Power Meter Settings dialog on the PNA. Changing certain values from that dialog will change values of the corresponding properties on this COM object.

**VB Syntax** *pwrCal*.LaunchPowerMeterSettingsDialog

**Variable** (Type) - Description

*pwrCal* A SourcePowerCalibrator (**object**)

**Return Type** None

**Default** Not Applicable

**Examples** `powerCalibrator.LaunchPowerMeterSettingsDialog`

**C++ Syntax** HRESULT put\_LaunchPowerMeterSettingsDialog();

**Interface** ISourcePowerCalibrator2

Write only

## LoadFile Method

---

**Description** Loads a previously-configured mixer attributes file (.mxr)

**VB Syntax** *mixer*.LoadFile (*filename*)

**Variable** **(Type) - Description**

*mixer* A IMixer Interface pointer to the Meas **(object)**

*filename* (String) Full path, file name, and .mxr extension of the mixer attributes file.  
Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents".

**Return Type** String

**Default** Not Applicable

**Examples** `mixer.LoadFile ("C:\Program Files\Agilent\Network Analyzer\Documents\myMixer.mxr")`

**C++ Syntax** HRESULT put\_LoadFile(BSTR newVal)

**Interface** IMixer

Write-only

**ManualTrigger Method**

---

**Description** Triggers the analyzer when `TriggerSignal = naTriggerManual`.

**Note:** An **SMC Fixed Output** measurement cannot be triggered using this command. For more information, see the [example program](#).

**VB Syntax** `app.ManualTrigger [sync],[timeout]`

**Variable (Type) - Description**

*app* An [Application](#) (**object**)

*sync* (**boolean**) - Optional argument.  
A variable set to either True or False.

**True** - The analyzer waits until the trigger is completed to process subsequent commands.

**False** - Subsequent commands are processed immediately (the default setting)

*timeout* (**long**) - Optional argument.  
If *sync* is true, *timeout* sets the amount of time the PNA will wait until continuing program execution. Units are milliseconds. A value of -1 (the default setting) causes the PNA to wait indefinitely.

If *sync* is False, the timeout setting is ignored.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
' After Manual trigger is executed, the PNA will wait 1 second
to continue program execution
Dim wait as Boolean
wait = True
app.ManualTrigger wait, 1000
```

**C++ Syntax** `HRESULT ManualTrigger(VARIANT_BOOL bSynchronize, long timeout)`

**Interface** `IApplication`

## MessageText Property

---

**Description** Returns text for the specified eventID

**VB Syntax** `app.MessageText,eventID,message`

**Variable** **(Type) - Description**

*app* An [Application](#) **(object)**

*eventID* **(enum naEventID)** Choose from the list in [Working with the Analyzer's Events](#)

*message* **(string)** - variable to store the returned message

**Return Type** String

**Default** Not Applicable

**Examples** `RFNA.MessageText naEventID_ARRANGE_WINDOW_EXCEED_CAPACITY,  
message`

**C++ Syntax** HRESULT get\_MessageText( tagNAEventID msgID, BSTR\* message)

**Interface** IApplication



Write-only

**NextIFBandwidth Method**

---

**Description** A function that returns the Next higher IF Bandwidth value. Use to retrieve the list of available IFBandwidth settings.

**VB Syntax** `chan.Next_IFBandwidth bw`

**Variable** **(Type) - Description**

*chan* A Channel **(object)**

*bw* **(double)** - The argument that you use to send an IFBandwidth. The function uses this argument to return the Next higher IFbandwidth.

**Return Type** Double

**Default** Not Applicable

**Examples**

```
Public pnbw As Double 'declare variable outside of procedure
pnbw = chan.IFBandwidth 'put the current IFBW in pnbw
chan.Next_IFBandwidth pnbw 'function returns the Next higher
IFBandwidth.
chan.IFBandwidth = pnbw 'set IFBW to the Next value
```

**C++ Syntax** HRESULT Next\_IFBandwidth (double \*pVal)

**Interface** IChannel

Write-only

## NumberOfGroups Method

---

**Description** Sets the Number of trigger signals the channel will receive. After the channels has received that number of trigger signals, the channel switches to Hold mode.

To begin sweeping the number of groups, send app.Continuous

**VB Syntax** *chan.NumberOfGroups num, sync*

**Variable** (Type) - Description

*chan* A Channel (**object**)

*num* (**long integer**) Number of trigger signals the channel will receive. Choose any number between 1 and 2 million

*sync* (**boolean**)

Variable set to either:

**True** - subsequent commands are not processed until the groups are complete. **Do not use with manual trigger.**

**False** - subsequent commands are processed immediately

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `chan.NumberOfGroups`

**C++ Syntax** HRESULT NumberOfGroups(long count, VARIANT\_BOOL bWait)

**Interface** IChannel

**OpenCalSet Method OBSOLETE**

**Description** This command is no longer necessary. The CalSet.get... and put... commands that required this command have been replaced.

Open the Cal Set to read/write a particular **CalType**. Learn more about [reading and writing Cal Data using COM](#).

This method is a prerequisite to several other Cal Set methods.

A Cal Set can contain more than one CalType. This method opens the Cal Set and allows access to a particular set of terms. Subsequent commands like [getErrorTerm](#) use this information to access the correct error terms in the Cal Set. For example:

```
cset.OpenCalSet (naCalType_TwoPortSOLT,3,2)
cset.PutErrorTerm(naDirectivity, 1, 1, Buffer)
```

The directivity error term for port 1 could belong to any number of caltypes: Full1Port (S11), Full2Port (12), Full2Port (13) or Full3Port (123). The **CalType and port** specifiers in OpenCalSet directs the uploaded directivity term to the correct set of error terms.

To close the Cal Set, see [CloseCalSet](#).

**VB Syntax** *CalSet.OpenCalSet (CalType, p1, p2, p3)*

**Variable (Type) - Description**

*CalSet* **(object)** - A Cal Set object

*CalType* (enum as naCalType) - type of correction to be applied. Choose from:

| <b>Caltype</b>                               | <b>p arguments required</b>       |
|----------------------------------------------|-----------------------------------|
| <b>0</b> - naCalType_Response_Open           | p1                                |
| <b>1</b> - naCalType_Response_Short          | p1                                |
| <b>2</b> - *naCalType_Response_Thru          | p1 (rcv), p2 (src)                |
| <b>3</b> - *naCalType_Response_Thru_And_Isol | p1 (rcv), p2 (src)                |
| <b>4</b> - naCalType_OnePort                 | p1                                |
| <b>5</b> - naCalType_TwoPort_SOLT            | p1, p2                            |
| <b>6</b> - naCalType_TwoPort_TRL             | p1, p2                            |
| <b>7</b> - naCalType_None                    | N/A                               |
| <b>8</b> - naCalType_ThreePort_SOLT          | p1, p2, p3                        |
| <b>9</b> - Custom                            | N/A                               |
| <b>10</b> - naCalType_FourPort_SOLT          | p1, p2, p3<br>(port 4 is assumed) |

\* order of port arguments is significant for these CalTypes

*p1* **(long)** - required. This argument must be specified.

This specifies either:

- the one significant port for an open/short response cal or a 1 port cal.
- or one of the ports involved in a 2 or 3 port cal
- or the **receive** port for a thru response / thru-isolation cal.

*p2* **(long)** - required for any caltype involving more than one port

This specifies either:

- one of the ports involved in a 2 or 3 port cal (order independent)
- or the **source** port for a thru response / thru-isolation cal

*p3* **(long)** - required only for 3 port cal

This specifies either:

- one of the ports involved in a 3 port cal (order independent)

**Return Type** None

**Default** Not Applicable

**Examples** `CalSet.OpenCalSet naCalType_ThreePort_SOLT, 3,2,1`

**C++ Syntax** HRESULT OpenCalSet ( naCalType, port1, [optional] port2, [optional] port3);

**Interface** ICalSet

## Write-Read

**Parse Method**

---

**Description** Executes a SCPI command.

**VB Syntax** `scpi.Parse ("SCPI command")`

**Variable** **(Type) - Description**

`scpi` A ScpiStringParser (**object**)

*SCPI command* (**string**) - Any valid SCPI command

**Return Type** String

**Default** Not Applicable

**Examples**

```
Dim scpi As ScpiStringParser
Set scpi = app.ScpiStringParser
Dim startfreq As Double
startfreq = 100e6
'
scpi.Parse ("Sens:Freq:Start " & startfreq)'Write

Dim str As String
str = scpi.Parse ("Sens:Freq:Start?")'Read
```

**C++ Syntax** HRESULT Parse(BSTR SCPI\_Command, BSTR \*pQueryResponse)

**Interface** IScpiStringParser

## Preset Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                             |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Application Object:</b> Deletes all traces and windows. In addition, resets the analyzer to factory defined default settings and creates an S11 measurement named "CH1_S11_1" in window 1.<br><b>Channel Object:</b> Resets the channel (object) to factory defined default settings. Does NOT delete the current measurements or add a new measurement. |
| <b>VB Syntax</b>   | <i>app.Preset</i><br><i>chan.Preset</i>                                                                                                                                                                                                                                                                                                                     |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                 |
| <i>app</i>         | An <u>Application</u> ( <b>object</b> )                                                                                                                                                                                                                                                                                                                     |
| <i>chan</i>        | A Channel ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                 |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                              |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                              |
| <b>Examples</b>    | <code>app.Preset</code>                                                                                                                                                                                                                                                                                                                                     |
| <b>C++ Syntax</b>  | HRESULT Preset()                                                                                                                                                                                                                                                                                                                                            |
| <b>Interface</b>   | IApplication<br>IChannel                                                                                                                                                                                                                                                                                                                                    |

**PreviousIFBandwidth Method**

---

**Description** A function that returns the previous IF Bandwidth value. Use to retrieve the list of available IFBandwidth settings.

**VB Syntax** *chan.Previous\_IFBandwidth bw*

**Variable** (Type) - Description

*chan* A Channel **(object)**

*bw* **(double)** - The argument that you use to send an IFBandwidth. The function uses this argument to return the previous IFbandwidth.

**Return Type** Double

**Default** Not Applicable

**Examples**

```
Public pnbw As Double 'declare variable outside of procedure
PreBW = chan.IFBandwidth 'put the current IFBW in PreBW
chan.Previous_IFBandwidth PreBW 'function returns the Previous
IFBandwidth of the current one.
chan.IFBandwidth = PreBW 'set IFBW to the previous value
```

**C++ Syntax** HRESULT Previous\_IFBandwidth (double \*pVal)

**Interface** IChannel

Write-only

## PrintToFile Method

---

**Description** Saves the screen image to a bitmap file.

**VB Syntax** `app.PrintToFile filename`

**Variable (Type) - Description**

*app* An Application (**object**)

*filename* (**string**) Full path, file name, and extension of the screen image file.

Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents".

Use one of the following extensions:

- .bmp - not recommended due to large file size
- .jpg - not recommended due to poor quality
- **.png - recommended**

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.PrintToFile "C:\Program Files\Agilent\Network Analyzer\Documents\myfile.png"`

**C++ Syntax** HRESULT PrintToFile(BSTR bstrFile)

**Interface** IApplication



## PutComplex Method

---

**Description** Puts real and imaginary data into the specified location. This method forces the channel into Hold mode to prevent the input data from being overwritten. Learn more about [reading and writing Cal Data using COM](#).

Data put in the raw data store will be **re-processed** whenever a change is made to the measurement attributes such as format or correction.

Data put in the measurement results store will be **overwritten** by any measurement attribute changes.

See also [putNAComplex](#)

**VB Syntax** *measData.putComplex location, numPts, real(), imag(), [format]*

**Variable (Type) - Description**

*measData* An IArrayTransfer interface which supports the Measurement object

*location* **(enum NADataStore)** Where the Data will be put. Choose from:

0 - naRawData

1 - naCorrectedData

2 - naMeasResult

3 - naRawMemory

4 - naMemoryResult

5 - naDivisor - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using [DataToDivisor Method](#).

*numPts* **(long integer)** - Number of data points in the channel

*real()* **(single)** - Array containing real data values

*imag()* **(single)** - Array containing imaginary data values

*format* **(enum NADataFormat)** optional argument - display format of the real and imaginary data. Only used if destination is naMeasResult or naMemoryResult buffer. If unspecified, data is assumed to be in naDataFormat\_Polar

0 - naDataFormat\_LinMag

1 - naDataFormat\_LogMag

2 - naDataFormat\_Phase

3 - naDataFormat\_Polar

4 - naDataFormat\_Smith

5 - naDataFormat\_Delay

6 - naDataFormat\_Real

7 - naDataFormat\_Imaginary

8 - naDataFormat\_SWR

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
Dim measData As IArrayTransfer
Set measData = app.ActiveMeasurement

measData.putComplex naMemoryResult, 201,
real(0), imag(0), naDataFormat_SWR
```

**C++ Syntax** HRESULT putComplex( tagNADataStore DataStore, long INumValues, float\* pReal, float\* plmag, tagDataFormat displayFormat)

**Interface** IArrayTransfer

## PutDataComplex Method

---

**Description** Puts complex data into the specified location. This method forces the channel into Hold mode to prevent the input data from being overwritten.

**VB Syntax** *meas.putDataComplex location, data*

**Variable** **(Type) - Description**

*meas* A measurement **(object)**

*location* **(enum NADataStore)** Where the Data will be put. Choose from:

0 - naRawData

1 - naCorrectedData

2 - naMeasResult

3 - naRawMemory

4 - naMemoryResult

5 - naDivisor - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using [DataToDivisor Method](#).

- Data put in 0 - naRawData will be re-processed whenever a change is made to the measurement attributes such as format or correction.
- Data put in 2 - naMeasResult will be overwritten by any measurement attribute changes.
- When putting data into 3 - naRawMemory:
  1. Put the analyzer in hold mode
  2. Call [DataToMemory](#) to initialize a memory buffer
  3. Call putDataComplex(naRawMemory, data)

This ensures that the memory buffer is appropriately initialized before receiving new data.

*data* **(variant)** - A **two-dimensional** variant array.

---

**Note:** All buffers except naMeasResult and naMemoryResult require Complex data

---

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** ' Put 201 points worth of raw (complex) data into the measurement  
' Note that an array of complex numbers is represented by a 2-D array where the first rank is the number of points, and the 2nd rank is always size 2 (max index 1) representing the Real and Imag parts of the complex number.  
  
' complex array of data (2nd dimension of size 2 represents Re/Im  
Dim data(200,1) )  
For i = 0 to 200  
' Set Real part of data point i  
data(i,0) = i/200;  
' Set Imag part of data point i  
data(i,1) = i/200;  
Next  
app.ActiveMeasurement.putDataComplex naRawData, data

**C++ Syntax** HRESULT putDataComplex(tagNADataStore DataStore, VARIANT complexData)

**Interface** IMeasurement

Write-only

**PutErrorTerm Method - OBSOLETE**

**Description** **Note:** This command is replaced by [PutErrorTermByString](#)

Puts variant error term data into the error-correction buffer.

[Learn about reading and writing Calibration data.](#)

**VB Syntax** `cal.putErrorTerm(term,rcv, src, data)`

**Variable (Type) - Description**

*cal* A Calibrator (**object**)

*term* (**enum As NaErrorTerm**)  
 naErrorTerm\_Directivity\_Isolation  
 naErrorTerm\_Match  
 naErrorTerm\_Tracking

*rcv* (**long integer**) - Receiver Port

*src* (**long integer**) - Source Port

*data* (**variant**) Error term data in a two-dimensional array (0:1, 0:numpts-1).

| To get this             | Specify these parameters:  |            |            |
|-------------------------|----------------------------|------------|------------|
| Error Term              | <i>term</i>                | <i>rcv</i> | <i>src</i> |
| Fwd Directivity         | naET_Directivity Isolation | 1          | 1          |
| Rev Directivity         | naET_Directivity Isolation | 2          | 2          |
| Fwd Isolation           | naET_Directivity Isolation | 2          | 1          |
| Rev Isolation           | naET_Directivity Isolation | 1          | 2          |
| Fwd Source Match        | naErrorTerm_Match          | 1          | 1          |
| Rev Source Match        | naErrorTerm_Match          | 2          | 2          |
| Fwd Load Match          | naErrorTerm_Match          | 2          | 1          |
| Rev Load Match          | naErrorTerm_Match          | 1          | 2          |
| Fwd Reflection Tracking | naErrorTerm_Tracking       | 1          | 1          |
| Rev Reflection Tracking | naErrorTerm_Tracking       | 2          | 2          |
| Fwd Trans Tracking      | naErrorTerm_Tracking       | 2          | 1          |
| Rev Trans Tracking      | naErrorTerm_Tracking       | 1          | 2          |
| Fwd Trans Tracking      | naErrorTerm_Tracking       | 2          | 1          |

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `Dim varError As Variant  
varError = cal.putErrorTerm (naErrorTerm_Tracking,2,1,VarData)`

**C++ Syntax** HRESULT putErrorTerm(tagNAErrorTerm ETerm, long ReceivePort, long SourcePort, VARIANT varData)

**Interface** ICalibrator

**PutErrorTerm Method OBSOLETE**

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p>This command is <u>replaced</u> with <a href="#">PutErrorTermByString</a></p> <hr/> <p>Puts error term data into the Cal Set.</p> <p>Learn more about <a href="#">Reading and Writing Cal Data</a></p> <p>See examples of <a href="#">Reading</a> and <a href="#">Writing</a> Cal Set Data</p>                                                                              |
| <b>VB Syntax</b>   | <i>CalSet.putErrorTerm (term, rcv, src, data)</i>                                                                                                                                                                                                                                                                                                                              |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                    |
| <i>CalSet</i>      | <b>(Object)</b> A <a href="#">CalSet</a> Object                                                                                                                                                                                                                                                                                                                                |
| <i>term</i>        | <p><b>(enum As NaErrorTerm2)</b> Error Term. Choose from:</p> <ul style="list-style-type: none"> <li>0 - naET_Directivity (src = rcv)</li> <li>1 - naET_SourceMatch (src = rcv)</li> <li>2 - naET_ReflectionTracking (src = rcv)</li> <li>3 - naET_TransmissionTracking (src ≠ rcv)</li> <li>4 - naET_LoadMatch (src ≠ rcv)</li> <li>5 - naET_Isolation (src ≠ rcv)</li> </ul> |
| <i>rcv</i>         | <b>(long integer)</b> - Receiver Port                                                                                                                                                                                                                                                                                                                                          |
| <i>src</i>         | <b>(long integer)</b> - Source Port                                                                                                                                                                                                                                                                                                                                            |
| <i>data</i>        | <p><b>(variant)</b> Error term data in a two-dimensional array (0:1, 0:numpts-1). The data must be complex pairs.</p> <hr/> <p><b>Note:</b> See also <a href="#">PutErrorTermComplex</a> on the ICalData2 interface to avoid using the variant data type.</p> <hr/>                                                                                                            |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Examples</b>    | <a href="#">See an Example</a>                                                                                                                                                                                                                                                                                                                                                 |
| <b>C++ Syntax</b>  | HRESULT putErrorTerm(tagNAErrorTerm2 ETerm, long ReceivePort, long SourcePort, VARIANT varData)                                                                                                                                                                                                                                                                                |
| <b>Interface</b>   | ICalSet                                                                                                                                                                                                                                                                                                                                                                        |

## PutErrorTermByString

---

|                        |                                                                                                                                                                                                                                                                                                                                                            |
|------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b>     | Puts error term data into the Cal Set.<br>Learn more about <a href="#">Reading and Writing Cal Data</a><br>See examples of <a href="#">Reading</a> and <a href="#">Writing</a> Cal Set Data                                                                                                                                                                |
| <b>VB Syntax</b>       | <code>calSet.PutErrorTermByString(errorName, vdata)</code>                                                                                                                                                                                                                                                                                                 |
| <b>Variable</b>        | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                |
| <code>calSet</code>    | <b>(Object)</b> A <a href="#">CalSet</a> Object                                                                                                                                                                                                                                                                                                            |
| <code>errorName</code> | <b>(String)</b> The string name used to identify a particular error term in the Cal Set. An example string for port 3 directivity in a full 2 port cal might be "Directivity(3,3)". To determine the string names of error terms, see <a href="#">GetErrorTermList2</a> .                                                                                  |
| <code>vdata</code>     | <b>(Variant)</b> This data array is usually two dimensional. Each element is a type single. The two elements represent the real and imaginary parts of a complex pair.<br><hr/> <b>Note:</b> This structure is compatible with scripting clients who can only use variants. For alternative methods that use typed arrays, see <a href="#">ICalData3</a> . |
| <b>Return Type</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                             |
| <b>Default</b>         | Not Applicable                                                                                                                                                                                                                                                                                                                                             |
| <b>Examples</b>        | <a href="#">See an Example</a>                                                                                                                                                                                                                                                                                                                             |
| <b>C++ Syntax</b>      | <code>HRESULT PutStandardByString( BSTR bufferName, VARIANT vardata)</code>                                                                                                                                                                                                                                                                                |
| <b>Interface</b>       | ICalSet2                                                                                                                                                                                                                                                                                                                                                   |



**PutErrorTermComplex Method OBSOLETE**

|                    |                                                                                                                                                                                                                                                  |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This command is replaced by <a href="#">PutErrorTermComplexByString</a><br><br>Puts error term data into the error-correction data buffer. Learn more about <a href="#">reading and writing Cal data using COM</a>                  |
| <b>VB Syntax</b>   | <code>data.putErrorTermComplex term, rcv, src, numPts, real(), imag()</code>                                                                                                                                                                     |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                      |
| <i>data</i>        | An ICalData pointer to the Calibrator object                                                                                                                                                                                                     |
| <i>term</i>        | <b>(enum NAErrorTerm)</b> - The error term to be retrieved. Choose from: <ul style="list-style-type: none"> <li>• <b>naErrorTerm_Directivity_Isolation</b></li> <li>• <b>naErrorTerm_Match</b></li> <li>• <b>naErrorTerm_Tracking</b></li> </ul> |
| <i>rcv</i>         | <b>(long integer)</b> - Receiver Port                                                                                                                                                                                                            |
| <i>src</i>         | <b>(long integer)</b> - Source Port                                                                                                                                                                                                              |
| <i>numPts</i>      | <b>(long integer)</b> - number of data points in the array                                                                                                                                                                                       |
| <i>real()</i>      | <b>(single)</b> - array containing the <b>real</b> part of the calibration data. One-dimensional: the number of data points.                                                                                                                     |
| <i>imag()</i>      | <b>(single)</b> - array containing the <b>imaginary</b> part of the calibration data. One-dimensional: the number of data points.                                                                                                                |

| To get this             | Specify these parameters:  |            |            |
|-------------------------|----------------------------|------------|------------|
| Error Term              | <i>term</i>                | <i>rcv</i> | <i>src</i> |
| Fwd Directivity         | naET_Directivity Isolation | 1          | 1          |
| Rev Directivity         | naET_Directivity Isolation | 2          | 2          |
| Fwd Isolation           | naET_Directivity Isolation | 2          | 1          |
| Rev Isolation           | naET_Directivity Isolation | 1          | 2          |
| Fwd Source Match        | naErrorTerm_Match          | 1          | 1          |
| Rev Source Match        | naErrorTerm_Match          | 2          | 2          |
| Fwd Load Match          | naErrorTerm_Match          | 2          | 1          |
| Rev Load Match          | naErrorTerm_Match          | 1          | 2          |
| Fwd Reflection Tracking | naErrorTerm_Tracking       | 1          | 1          |
| Rev Reflection Tracking | naErrorTerm_Tracking       | 2          | 2          |
| Fwd Trans Tracking      | naErrorTerm_Tracking       | 2          | 1          |

|                          |                                                                                                                                                     |                      |   |   |
|--------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------|----------------------|---|---|
|                          | Rev Trans Tracking                                                                                                                                  | naErrorTerm_Tracking | 1 | 2 |
|                          | Fwd Trans Tracking                                                                                                                                  | naErrorTerm_Tracking | 2 | 1 |
| <b>Return Type</b>       | Not Applicable                                                                                                                                      |                      |   |   |
| <b>Default</b>           | Not Applicable                                                                                                                                      |                      |   |   |
| <b>Examples</b>          | <pre>Dim eData As ICalData Set eData = chan.Calibrator eData.putErrorTermComplex naErrorTerm_Directivity_Isolation, 1, 1, 201, rel(0), img(0)</pre> |                      |   |   |
| <b><u>C++</u> Syntax</b> | HRESULT putErrorTermComplex(tagNAErrorTerm ETerm, long ReceivePort, long SourcePort, long* pNumValues, float* pReal, float* plmag)                  |                      |   |   |
| <b>Interface</b>         | ICalData                                                                                                                                            |                      |   |   |

**PutErrorTermComplex Method** OBSOLETE

|                     |                                                                                                                                                                                                                                             |
|---------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b>  | This command is <u>replaced</u> with <u>PutErrorTermComplexByString</u><br>Puts error term data into the Cal Set.<br>Learn more about <u>Reading and Writing Cal Data</u><br>See examples of <u>Reading</u> and <u>Writing</u> Cal Set Data |
| <b>VB Syntax</b>    | <code>data.putErrorTermComplex term, rcv, src, numPts, real(), imag()</code>                                                                                                                                                                |
| <b>Variable</b>     | <b>(Type) - Description</b>                                                                                                                                                                                                                 |
| <code>data</code>   | An <u>ICalData2</u> pointer to a Cal Set object                                                                                                                                                                                             |
| <code>term</code>   | <b>(enum NAErrorTerm2)</b> - The error term to be written. Choose from:<br>0 - naET_Directivity<br>1 - naET_SourceMatch<br>2 - naET_ReflectionTracking<br>3 - naET_TransmissionTracking<br>4 - naET_LoadMatch<br>5 - naET_Isolation         |
| <code>rcv</code>    | <b>(long)</b> - Receiver Port                                                                                                                                                                                                               |
| <code>src</code>    | <b>(long)</b> - Source Port                                                                                                                                                                                                                 |
| <code>numPts</code> | <b>(long)</b> - number of data points in the real and imaginary arrays.                                                                                                                                                                     |
| <code>real()</code> | <b>(single)</b> - array containing the <b>real</b> part of the calibration data. One-dimensional: the number of data points.                                                                                                                |
| <code>imag()</code> | <b>(single)</b> - array containing the <b>imaginary</b> part of the calibration data. One-dimensional: the number of data points.                                                                                                           |
| <b>Return Type</b>  | Not Applicable                                                                                                                                                                                                                              |
| <b>Default</b>      | Not Applicable                                                                                                                                                                                                                              |
| <b>Examples</b>     | <pre>Dim eData As ICalData2 Set eData = app.GetCalManager.Cal Sets.Item(1) eData.putErrorTermComplex naET_LoadMatch, 1, 2, numpts, rel(0), img(0)</pre>                                                                                     |
| <b>C++ Syntax</b>   | <code>HRESULT putErrorTermComplex(tagNAErrorTerm2 ETerm, long ReceivePort, long SourcePort, long* pNumValues, float* pReal, float* plmag)</code>                                                                                            |
| <b>Interface</b>    | ICalData2                                                                                                                                                                                                                                   |

## PutErrorTermComplexByString Method

---

**Description** Puts error term data into the Cal Set.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

**VB Syntax** *ICalData3.PutErrorTermComplexByString* *errorName, InumPoints, real(0), imag(0)*

**Variable (Type) - Description**

*ICalData3* An [ICalData3](#) pointer to a Cal Set object.

*errorName* **(String)** The string name used to identify a particular error term in the Cal Set. An example string for port 3 directivity in a full 2 port cal might be "Directivity(3,3)". To determine the string names of error terms, see [GetErrorTermList2](#).

*InumPoints* **(Long)** The number of data points in the real and imaginary arrays.

*real* **(Single)** The real component of the complex data.

*imag* **(Single)** The imaginary component of the complex data.

---

**Note:** The size of the real and imaginary arrays should be the same.

---

**Return Value** Not Applicable

**Default** Not Applicable

**Examples** [See example](#)

**C++ Syntax** HRESULT PutErrorTermComplexByString( BSTR bufferName, long InumPoints, float\* real, float\* imag);

**Interface** ICalData3

**PutScalar Method**

---

**Description** Puts Scalar data in the Measurement Result buffer. The putScalar array is not processed by the analyzer; it is just displayed. Any change to the measurement state (changing the format, for example) will cause the putScalar data to be overwritten with the data processed from the raw data buffer.

**VB Syntax** *measData.putScalar, format, numPts, data*

**Variable** (Type) - Description

*measData* An IArrayTransfer interface which supports the Measurement object.

*format* **(enum NADataFormat)** Format of the data. Choose from:

- 0 - naDataFormat\_LinMag
- 1 - naDataFormat\_LogMag
- 2 - naDataFormat\_Phase
- 5 - naDataFormat\_Delay
- 6 - naDataFormat\_Real
- 7 - naDataFormat\_Imaginary
- 8 - naDataFormat\_SWR

---

**Note: Smith and Polar** formats are not allowed.

---

*numPts* **(integer)** - Number of values. Usually the number of points in the trace (chan.NumberOfPoints).

*data* **(single)** - A one-dimensional array of Scalar data matching the number of points in the current measurement.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
Dim measData As IArrayTransfer
Set measData = app.ActiveMeasurement

measData.putScalar naDataFormat_LogMag, 201, dScalar(0)
```

**C++ Syntax** HRESULT putScalar(tagDataFormat eFormat, long INumValues, float\* pArrayOfScalar)

**Interface** IArrayTransfer

## PutNAComplex Method

---

**Description** Puts complex data into the specified location. This method forces the channel into Hold mode to prevent the input data from being overwritten. The data is processed and displayed.

Data put in the naRawData store will be **re-processed** whenever a change is made to the measurement attributes such as format or correction.

Data put in the naMeasResult store will be **overwritten** by any measurement attribute changes (such as moving a marker).

---

**Note:** This method uses NAComplex which is a user-defined data type. If you cannot or prefer not to use this data type, use the [putComplex](#) method.

---

**VB Syntax** *measData.putNAComplex location, numPts, data, [format]*

**Variable** **(Type) - Description**

*measData* An IArrayTransfer interface which supports the Measurement object

*location* **(enum NADataStore)** Where the Data will be put. Choose from:

0 - naRawData

1 - naCorrectedData

2 - naMeasResult

3 - naRawMemory

4 - naMemoryResult

5 - naDivisor - When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace using [DataToDivisor Method](#).

*numPts* **(long integer)** - Number of data points in the channel

*data* **(NAComplex)** - A one-dimensional array of Complex data matching the number of points in the current measurement.

*format* **(enum NADisplayFormat)** - Optional argument. Format of the data. If unspecified, naDataFormat\_Polar is assumed. Only used when the destination store is naMeasResult or naMemoryResult.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
Dim measData As IArrayTransfer
Set measData = app.ActiveMeasurement

measData.putNAComplex naMemoryResult, 201, dRawComplex(0)
```

**C++ Syntax** HRESULT putNAComplex(tagNADataStore DataStore, long INumValues, TsComplex\* pArrayOfComplex, tagDataFormat displayFormat)

**Interface** IArrayTransfer



**put\_Output Method**

---

**Description** Writes a TTL HI or TTL Low to output pins 3 or 4 of the Material Handler IO connector.

Each pin also has a latched output which is written to with USER. With the latched (USER) outputs, the value is not applied to the associated pin until a positive edge is detected at INPUT1 (pin 2).

**VB Syntax** `handlerIo.put_Output (pin) = value`

**Variable** **(Type) - Description**

*handlerIo* **(object)** - A HandlerIO object

*pin* **(enum as NAMatHandlerOutput)** - pin to write data to. Choose from:

**naOutput1 - (0)** - pin3

**naOutput1User (1)** - pin3 latched (applied to pin 3 on positive edge of Input1-pin2)

**naOutput2 (2)** - pin4

**naOutput2User (3)** - pin4 latched (applied to pin 4 on positive edge of Input1-pin2)

*value* **(Variant)** Value to write to the selected pin. Choose from

**0** - TTL LOW

**1** - TTL HIGH

**Return Type** Not Applicable

**Default** 0

**Examples** `handlerIo.put_Output(naOutput1)= 1`

**C++ Syntax** `HRESULT put_Output ( tagNAMatHandlerOutput Output, VARIANT Data );`

**Interface** IHWMaterialHandlerIO



## put\_OutputVoltage Method

---

- Description** Writes voltages on the DAC/Analog Output 1 and Output 2 (pins 2 and 3 of the Aux I/O connector)
- VB Syntax** *AuxIO.put\_OutputVoltage output, voltage*
- Variable (Type) - Description**
- AuxIO* **(object)** - A Hardware Auxiliary Input / Output object
- output* **(variant)** Number of the output DAC to write voltage to. Choose from:  
1 Output DAC 1 - (pin 2)  
2 Output DAC 2 - (pin 3)
- voltage* **(double)** Voltage to write to the output DAC. Choose a voltage from -10 to 10
- Return Type** None
- Default** None
- Examples** `HWAuxIO.put_OutputVoltage 1,9 'set Analog Out1 to +9v`
- C++ Syntax** HRESULT put\_OutputVoltage (VARIANT Output, double Voltage );
- Interface** IHWAuxIO

Write-only

## put\_OutputVoltageMode Method

---

**Description** This command sets the mode of the selected "Analog Out" line on the Auxiliary IO connector. The modes give the user the option to have the requested voltage applied immediately or not until the sweep is done. To read the mode on each output use get\_OutputVoltageMode Method.

**VB Syntax** *auxIo.put\_OutputVoltageMode (output, mode)*

**Variable** **(Type) - Description**

*auxIo* **(Object)** An AuxIO object

*output* Analog Output to receive mode setting. Choose from **1** or **2**

*mode* **(enum NAOutputVoltageMode)**

**naWaitEOS** - While in this mode any voltage changes sent to the selected analog out will only get applied to the output between sweeps.

**naNoWait** - While in this mode any voltage changes sent to the selected analog out will occur right away without waiting until the end of a sweep, the voltage gets applied immediately.

**Return Type** NAOutputVoltageMode

**Default** naWaitEOS

**Examples** `auxIo.put_OutputVoltageMode 1, naWaitEOS 'Write`

**C++ Syntax** HRESULT put\_OutputVoltageMode(VARIANT Output, tagNAOutputVoltageMode dNewMode);

**Interface** IHWAuxIO

## put Port Method

**Description** Writes a value to the specified port. Use the get\_Port Method to read the settings from the "readable" ports (C, D, E).

**VB Syntax** *handlerIo.put\_Port (port) = value*

**Variable (Type) - Description**

*handlerIo* **(object)** - A HandlerIO object

*port* **(enum as NAMatHandlerPort)** - port to put data into. Choose from:

**naPortA - (0)**

**naPortB - (1)**

**naPortC - (2)**

**naPortD - (3)**

**naPortE - (4)**

**naPortF - (5)**

**naPortG - (6)**

**naPortH - (7)**

*value* The number of the data bits to set. The following table shows what the *value* represents:

**Note:** When writing to port G, port C must be set to output mode

When writing to port H, both port C and port D must be set to output mode. Use Port Mode Property

| Port | Max allowable <num> | MSB.....LSB<br>23.....0               |            |
|------|---------------------|---------------------------------------|------------|
| A    | 255                 | A7...A0                               | Write-only |
| B    | 255                 | B7...B0                               | Write-only |
| C    | 15                  | C3...C0                               | Read-Write |
| D    | 15                  | D3...D0                               | Read-Write |
| E    | 255                 | D3...D0 + C3...C0                     | Read-Write |
| F    | 65535               | B7...B0 + A7...A0                     | Write-only |
| G    | 1048575             | C3...C0 + B7...B0 + A7...A0           | Write-only |
| H    | 16777215            | D3...D0 + C3...C0 + B7...B0 + A7...A0 | Write-only |

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `handlerIo.put Port(naPortB)= 15`

**C++ Syntax** HRESULT put\_Port ( tagNAMatHandlerPort Port, VARIANT Data );

**Interface** IHWMaterialHandlerIO

**put\_PortCData Method**

---

**Description** Writes a 4-bit value to Port C on the Aux I/O connector (pins 22-25) and the Material Handler IO (pins 21-24 Anritsu) - (pins 22-25 Avantest).

**Note:** These lines are connected to both the Handler IO and Aux IO in the PNA. Therefore, this command will affect both of these connectors in the same way.

**VB Syntax** *AuxIO.put\_PortCData num*

**Variable** **(Type) - Description**

*AuxIO* **(object)** - A Hardware Auxiliary Input / Output object

*num* **(variant)** - 4 bit binary value. Choose from 0-15

**Return Type** None

**Default** None

**Examples** `HWAuxIO.put_PortCData 15 'If Positive Logic, Port C lines C0, C1, C2, C3 go High. If Negative Logic, they go Low.`

**C++ Syntax** `HRESULT put_PortCData( VARIANT Data );`

**Interface** IHWAuxIO

## PutDataScalar Method

---

**Description** Puts formatted variant scalar data into the measurement result buffer. The data will be immediately processed and displayed. Subsequent changes to the measurement state will be reflected on the display.

Always precede this command by setting the format on the measurement to be consistent with the format of the data being sent to the analyzer. In this way, the display annotation will be correct.

Execution of this command does not change the display format.

**VB Syntax** *meas.putDataScalar format, data*

**Variable** (Type) - Description

*meas* A measurement (**object**)

*format* (**enum NADataFormat**) Format of the data. **This value is presently ignored by the PNA.** Data is always presented in the current format.

Choose from:

- 0 - naDataFormat\_LinMag
- 1 - naDataFormat\_LogMag
- 2 - naDataFormat\_Phase
- 3 - naDataFormat\_Polar
- 4 - naDataFormat\_Smith
- 5 - naDataFormat\_Delay
- 6 - naDataFormat\_Real
- 7 - naDataFormat\_Imaginary
- 8 - naDataFormat\_SWR

**Notes:**

- The getData (variant) method includes a "format" argument, which allows scalar (one-dimensional) data. To put data back into the "raw" data buffer using this (putDataComplex) method, specify **Polar** format when using the getData method.
- **Phase** format accepts data in radians (not degrees) and displays in degrees. To convert to degrees: radians \* (57.29577951308233) = degrees. The getData method returns degrees if the request is for phase data.

*data* (**variant**) - A 1-dimension array of single precision floating point numbers.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
' Put 201 points worth of scalar data into the measurement
' 200 is max index, so 0 to 200 is 201 points
Dim data(200) ' array of 201 (scalar) data points
' Fill the array
For i = 0 to 200
data(i) = i/200;
Next
app.ActiveMeasurement.putDataScalar 0, data
```

**C++ Syntax** HRESULT putDataScalar(tagNADataStore DataStore, VARIANT scalarArray)

**Interface** IMeasurement

## PutShortcut Method

---

|                    |                                                                                                                                                                                        |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Defines a Macro (shortcut) file in the analyzer. This command links a file name and path to the Macro file. The file must be put in the PNA at the location indicated by this command. |
| <b>VB Syntax</b>   | <i>app.PutShortcut index,title,path</i>                                                                                                                                                |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                            |
| <i>app</i>         | An <u>Application</u> ( <b>object</b> )                                                                                                                                                |
| <i>index</i>       | <b>(long)</b> - Number of the macro to be stored in the analyzer. If the index number already exists, the existing macro is replaced with the new macro.                               |
| <i>title</i>       | <b>(string)</b> - The name to be assigned to the macro                                                                                                                                 |
| <i>path</i>        | <b>(string)</b> - Full path, file name, and extension of the existing macro "executable" file.                                                                                         |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                         |
| <b>Default</b>     | Not Applicable                                                                                                                                                                         |
| <b>Examples</b>    | <code>app.PutShortcut 1,"Test","C:\Automation\MyTest.vbs"</code>                                                                                                                       |
| <b>C++ Syntax</b>  | HRESULT PutShortcut(long Number, BSTR title, BSTR pathname)                                                                                                                            |
| <b>Interface</b>   | IApplication                                                                                                                                                                           |



**putSourcePowerCalDataEx Method**


---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p><b>Note:</b> This method replaces <a href="#">putSourcePowerCalData Method</a></p> <p>Inputs source power calibration data (as variant data type) to this channel for a specific source port.</p> <p>If the channel is sweeping the source backwards, then the first data point is the highest frequency value; the last data point is the lowest. Use the <a href="#">Get X-Axis Values</a> command to return the X-axis values in the displayed order.</p> <p>The calibration is not valid if the current number of points on the channel is not equal to the number of values that were input.</p> <hr/> <p><b>Note:</b> This method sends variant data which is less efficient than methods available on the <a href="#">ISourcePowerCalData</a> interface.</p> <hr/> |
| <b>VB Syntax</b>   | <code>chan.putSourcePowerCalData buffer, sourcePort, data</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
|                    | <code>chan</code> <b>(object)</b> – A Channel object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|                    | <code>buffer</code> <b>(enum NASourcePowerCalBuffer)</b> - The source power cal data buffer to write to.<br><b>0 - naCorrectionValues</b> This is the only data buffer currently available.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
|                    | <code>sourcePort</code> <b>(long integer)</b> – The source port for which calibration data is being requested.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
|                    | <code>data</code> <b>(variant)</b> – Array of source power cal data being input.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| <b>Return Type</b> | None                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <b>Examples</b>    | <code>chan.putSourcePowerCalDataEx naCorrectionValues, 1, varData</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>C++ Syntax</b>  | <code>HRESULT putSourcePowerCalDataEx(tagNASourcePowerCalBuffer bufSelect, long sourcePort, VARIANT varData);</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Interface</b>   | <code>IChannel4</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |

**putSourcePowerCalDataScalarEx Method**


---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p><b>Note:</b> This method replaces <a href="#">putSourcePowerCalDataScalar Method</a></p> <p>Inputs source power calibration data (as scalar values) to this channel for a specific source port.</p> <p>If the channel is sweeping the source backwards, then the first data point is the highest frequency value; the last data point is the lowest. Use the <a href="#">Get X-Axis Values2</a> command to return the X-axis values in the displayed order.</p> |
| <b>VB Syntax</b>   | <i>chanData.putSourcePowerCalDataScalarEx buffer, sourcePort, numValues, data</i>                                                                                                                                                                                                                                                                                                                                                                                  |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| <i>chanData</i>    | <b>(interface)</b> – An <a href="#">ISourcePowerCalData2</a> interface on the Channel (object)                                                                                                                                                                                                                                                                                                                                                                     |
| <i>buffer</i>      | <b>(enum NASourcePowerCalBuffer)</b> - The source power cal data buffer to write to.<br><b>0 - naCorrectionValues</b> This is the only buffer currently available.                                                                                                                                                                                                                                                                                                 |
| <i>sourcePort</i>  | <b>(long integer)</b> – The source port for which calibration data is being input.                                                                                                                                                                                                                                                                                                                                                                                 |
| <i>numValues</i>   | <b>(long integer)</b> – Number of data values being input.                                                                                                                                                                                                                                                                                                                                                                                                         |
|                    | <b>Note:</b> If this does not equal the current number of points on the channel, the calibration will not be valid.                                                                                                                                                                                                                                                                                                                                                |
| <i>data</i>        | <b>(single)</b> – Array of source power cal data being input.                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>Return Type</b> | None                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>Examples</b>    | <pre>Dim chanData As ISourcePowerCalData2 Set chanData = app.ActiveChannel chanData.putSourcePowerCalDataScalarEx naCorrectionValues, 1, 201, scalarCalValues(0)</pre>                                                                                                                                                                                                                                                                                             |
| <b>C++ Syntax</b>  | HRESULT putSourcePowerCalDataScalarEx(tagNASourcePowerCalBuffer bufSelect, long sourcePort, long numValues, float *pData);                                                                                                                                                                                                                                                                                                                                         |
| <b>Interface</b>   | ISourcePowerCalData2                                                                                                                                                                                                                                                                                                                                                                                                                                               |

**PutStandard Method OBSOLETE**

---

**Description** This command is replaced with [PutStandardByString](#)

Puts standard acquisition data into the Cal Set.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data.

**VB Syntax** *CalSet.putStandard class, rcv, src, data*

**Variable** **(Type) - Description**

*CalSet* **(object)** - A [Cal Set](#) object

*class* **(enum NACalClass)** Standard. Choose from:

1 - naClassA

2 - naClassB

3 - naClassC

4 - naClassD

5 - naClassE

6 - naReferenceRatioLine

7 - naReferenceRatioThru

**SOLT Standards**

1 - naSOLT\_Open

2 - naSOLT\_Short

3 - naSOLT\_Load

4 - naSOLT\_Thru

5 - naSOLT\_Isolation

**TRL Standards**

1 - naTRL\_Reflection

2 - naTRL\_Line\_Reflection

3 - naTRL\_Line\_Tracking

4 - naTRL\_Thru

5 - naTRL\_Isolation

*rcv* **(long)** - Receiver Port

*src* **(long)** - Source Port

*data* **(variant)** Error term data in a two-dimensional array (0:1, 0:numpts-1). The data must be complex pairs.

---

**Note:** See also [Put Standard Complex](#) on the ICalData2 interface to avoid using the variant data type.

---

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** [See an Example](#)

**C++ Syntax** HRESULT putStandard(tagNACalClass stdclass, long ReceivePort, long SourcePort, VARIANT varData)

**Interface** ICalSet

## PutStandardByString

---

**Description** Puts standard acquisition data into the Cal Set.  
Learn more about [Reading and Writing Cal Data](#)  
See examples of [Reading](#) and [Writing](#) Cal Set Data.

**VB Syntax** `PutStandardByString(stdName, vdata)`

**Variable** **(Type) - Description**

*stdName* **(String)** The string used to identify a particular standard in the Cal Set. An example string requesting the data for the Load standard in a full 2 port cal might be "S11C(3,3)".

*vdata* **(Variant)** The variant containing a safearray of variants. This data is usually two dimensional.

---

**Note:** The vardata array is a safearray of variants wrapped in a variant. This structure is compatible with scripting clients who can only use variants. For alternative methods that used typed arrays, see ICalData3.

---

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** [See an Example](#)

**C++ Syntax** `HRESULT PutStandardByString( BSTR bufferName, VARIANT vardata);`

**Interface** ICalSet2

**PutStandardComplex Method** **OBSOLETE**

**Description** This command is replaced with [PutStandardComplexByString](#)

Puts standards acquisition data into the Cal Set.

Learn more about [Reading and Writing Cal Data](#)

See examples of [Reading](#) and [Writing](#) Cal Set Data

**VB Syntax** *ICalData2.putStandardComplex class, rcv, src, numPts,real(),imag()*

**Variable** **(Type) - Description**

*ICalData2* An [ICalData2](#) pointer to the Cal Set object

*class* **(enum NACalClass)** Standard. Choose from:

1 - naClassA

2 - naClassB

3 - naClassC

4 - naClassD

5 - naClassE

6 - naReferenceRatioLine

7 - naReferenceRatioThru

**SOLT Standards**

1 - naSOLT\_Open

2 - naSOLT\_Short

3 - naSOLT\_Load

4 - naSOLT\_Thru

5 - naSOLT\_Isolation

**TRL Standards**

1 - naTRL\_Reflection

2 - naTRL\_Line\_Reflection

3 - naTRL\_Line\_Tracking

4 - naTRL\_Thru

5 - naTRL\_Isolation

*rcv* **(long)** - Receiver Port

*src* **(long)** - Source Port

*numPts* **(long)** - The number of data points in the real and imaginary arrays.

*real()* **(single)** - one-dimensional array containing the **real** part of the acquisition data.  
(0:points-1)

*imag()* **(single)** - one-dimensional array containing the **imaginary** part of the acquisition data.  
(0:points-1)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
Dim sdata As ICalData2
Set sdata = calmanager.CreateCal Set(1)
sdata.putStandardComplex naSOLT_Open, 1, 1, numpts, rel(0),
img(0)
```

**C++ Syntax** HRESULT putStandardComplex(tagNACalClass stdclass, long ReceivePort, long SourcePort, long INumValues, float\* pReal, float\* plmag)

**Interface** ICalData2

## PutStandardComplexByString

---

**Description** Puts standard acquisition data into the Cal Set.  
Learn more about [Reading and Writing Cal Data](#)  
See examples of [Reading](#) and [Writing](#) Cal Set Data.

**VB Syntax** `ICalData3.PutStandardComplexByString(stdName, InumPoints , real(o) , imag(0))`

**Variable (Type) - Description**

*ICalData3* An [ICalData3](#) pointer to a Cal Set object.

*stdName* **(String)** The string used to identify a particular standard in the Cal Set. An example string requesting the data for the Load standard in a full 2 port cal might be "S11C(3,3)".

*Inumpoints* **(long)** - The number of data points in the real and imaginary arrays.

*real* **(Single)** The real component of the complex data.

*imag* **(Single)** The imaginary component of the complex data.

**Return Value** Single

**Default** Not Applicable

**Examples** [See an Example](#)

**C++ Syntax** `HRESULT PutStandardComplexByString( BSTR bufferName, long InumPoints, float* real, float* imag);`

**Interface** ICalData3



Write-only

## Quit Method

---

**Description** Terminates the Network Analyzer application.

**VB Syntax** `app.Quit`

**Variable** **(Type) - Description**

`app` An Application (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.Quit`

**C++ Syntax** HRESULT Quit()

**Interface** IApplication

**Remarks** Under the rules of COM, the server should not exit until all references to it have been released. This method is a brute force way of terminating the application. Be sure to release all references (or terminate the client program) before attempting to restart the Network Analyzer application.

An alternate approach to terminating the application is to make the application invisible (`app.Visible = False`) and release all references. The server will shutdown.

## ReadData Method

---

- Description** Reads a 13-bit data word from the specified address. Data is read using the AD0 through AD12 lines of the external test set connector. The instrument generates the appropriate timing signals. It automatically controls timing signals LDS, LAS and RLW to strobe the address, and then read the data, from the external test set. See the [timing diagram](#) for Address and Data I/O read.
- VB Syntax** `value = ExtIO.ReadData (address)`
- Variable (Type) - Description**
- `value` **(variant)** - Variable to store the returned data
- `ExtIO` **(object)** - An ExternalTestSetIO object
- `address` **(variant)** - address to read data from.
- Return Type** Variant
- Default** Not Applicable
- Examples** `value = ExtIO.ReadData (15)`
- C++ Syntax** HRESULT ReadData (VARIANT Address, VARIANT\* Data);
- Interface** IHWExternalTestSetIO

**ReadRaw Method**

---

**Description** Reads a 16-bit value from the external test set. The 16-bit value is comprised of lines AD0 - AD12, Sweep Holdoff In and Interrupt In (inverted).

When this command is used the analyzer does NOT generate the appropriate timing signals; it simply reads the lines. The user needs to first use the WriteRaw method to do the initial setup. The RLW line (pin25) must be set to the appropriate level in order to read the test set connected.

**Below is the format of data that is read with ReadRaw:**

| Pin | Bit | Signal name                        |
|-----|-----|------------------------------------|
| 22  | 0   | AD0*                               |
| 23  | 1   | AD1*                               |
| 11  | 2   | AD2*                               |
| 10  | 3   | AD3*                               |
| 9   | 4   | AD4*                               |
| 21  | 5   | AD5*                               |
| 20  | 6   | AD6*                               |
| 19  | 7   | AD7*                               |
| 6   | 8   | AD8*                               |
| 5   | 9   | AD9*                               |
| 4   | 10  | AD10*                              |
| 17  | 11  | AD11*                              |
| 3   | 12  | AD12*                              |
| 2   | 13  | Sweep Holdoff In                   |
| 13  | 14  | Interrupt In (inverted internally) |
| na  | 15  | Always Zero, grounded internally   |

\*These lines are dependent on the state of RLW (pin25).  
Writing a 0(low) to RLW will set lines AD0-AD12 to write mode.  
Writing a 1(high) to RLW will set lines AD0-AD12 to read mode.

**VB Syntax** `value = ExtIO.ReadRaw (address)`

**Variable** **(Type) - Description**

`value` **(variant)** - Variable to store the returned data

`ExtIO` **(object)** - An External IO object

`address` **(variant)** - Address to read data from

**Return Type** Real

**Default** Not Applicable

**Examples** `value = ExtIO.ReadRaw (address)`

**C++ Syntax** HRESULT ReadRaw( VARIANT\* Input );

**Interface** IHWExternalTestSetIO

**Recall Method**

---

**Description** Recalls a measurement state, calibration state, or both, from the hard drive into the analyzer.

Use `app.Save` to save the measurement and calibration state.

**VB Syntax** `app.Recall (filename.ext)`

**Variable (Type) - Description**

`app` An Application (**object**)

`filename.ext` (**string**) - Full path, file name, and extension, of the file.

Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents"  
Use one of the following extensions:

- .sta - Instrument State
- .cal - Calibration file
- .cst - Both Instrument State and Calibration file
- .cti - Citifile (data will always be formatted. See Recalling Citifiles Using the PNA)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.Recall ("C:\Program Files\Agilent\Network Analyzer\Documents\MyState.cst")` 'Recalls "mystate.cst" from the specified folder

**C++ Syntax** `HRESULT Recall(BSTR bstrFile)`

**Interface** IApplication

Write-only

## Recall Kits Method

---

**Description** Recalls the calibration kits definitions that were stored with the SaveKits command.

**VB Syntax** `app.RecallKits`

**Variable** (Type) - Description

`app` An Application (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.RecallKits`

**C++ Syntax** HRESULT RecallKits()

**Interface** IApplication

Write-only

## Remove Method

---

**Description** Removes an item from a collection of objects.

**VB Syntax** *Object.Remove* *item*

**Variable** **(Type) - Description**

*Object* Any of the following **(objects)**

CalFactorSegments collection

Cal Sets collection

Measurements collection

NAWindows collection

PowerLossSegments collection

Segments collection

---

**Note:** Segments, CalFactorSegments, and PowerLossSegments have an OPTIONAL argument [size] referring to the number of segments to remove, starting with the *item* parameter.

---

*item* **(variant)** - Item number to be removed

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `Measurements.Remove 3 'Removes measurement 3`  
`segments.Remove 2,20 'Removes 20 segments (2 - 21)`

**C++ Syntax** HRESULT Remove(VARIANT index); //Measurements  
HRESULT Remove(VARIANT index); //Cal Sets  
HRESULT Remove(long windowNumber); //NAWindows  
HRESULT Remove(VARIANT index, long size); //Segments  
HRESULT Remove(VARIANT index, long size); //CalFactorSegments  
HRESULT Remove(VARIANT index, long size); //PowerLossSegments

**Interface** IMeasurements  
INAWindows  
ISegments  
ICalFactorSegments  
ICal Sets  
IPowerLossSegments

Write-only

**Reset Method**

---

|                    |                                                                                                                                 |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Removes all existing windows and measurements from the application. (Unlike <u>Preset</u> , does not create a new measurement.) |
| <b>VB Syntax</b>   | <code>app.Reset</code>                                                                                                          |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                     |
| <code>app</code>   | An <u>Application</u> ( <b>object</b> )                                                                                         |
| <b>Return Type</b> | Not Applicable                                                                                                                  |
| <b>Default</b>     | Not Applicable                                                                                                                  |
| <b>Examples</b>    | <code>app.Reset</code>                                                                                                          |
| <b>C++ Syntax</b>  | <code>HRESULT Reset()</code>                                                                                                    |
| <b>Interface</b>   | <code>IApplication</code>                                                                                                       |



Write-only

**RestoreCalKitDefaults Method**

---

**Description** Restores the original properties of the specified Cal Kit, overwriting the last definition with the factory defaults.

---

**NOTE:** ONLY works with PNA releases 1.0 through 1.6.

---

**VB Syntax** `app.RestoreCalKitDefaults (calKit)`

**Variable (Type) - Description**

*app* An Application (**object**)

*calKit* (**enum NACalKit**) - Calibration Kit to restore. Choose from:

- 1 - naCalKit\_85032F\_N50
- 2 - naCalKit\_85033E\_3\_5
- 3 - naCalKit\_85032B\_N50
- 4 - naCalKit\_85033D\_3\_5
- 5 - naCalKit\_85038A\_7\_16
- 6 - naCalKit\_85052C\_3\_5\_TRL
- 7 - naCalKit\_User7
- 8 - naCalKit\_User8
- 9 - naCalKit\_User9
- 10 - naCalKit\_User10

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.RestoreCalKitDefaults naCalKit_MechKit10`

**C++ Syntax** HRESULT RestoreCalKitDefaults\(\tagNACalKit kit)

**Interface** IApplication

## RestoreCalKitDefaultsAll Method

---

**Description** Restores the original properties of ALL of the Cal Kits, overwriting the last definitions with the factory defaults.

---

**NOTE:** ONLY works with PNA releases 1.0 through 1.6.

---

**VB Syntax** `app.RestoreCalKitDefaultsAll`

**Variable** **(Type) - Description**

`app` An Application (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.RestoreCalKitDefaultsAll`

**C++ Syntax** HRESULT RestoreCalKitDefaultsAll()

**Interface** IApplication

## Resume Method

---

|                    |                                                                                                                                                                                                                         |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Resumes the trigger mode of all channels that was in effect before sending the <a href="#">channels.Hold</a> method. Channels.Hold must be sent before channels.Resume, using the same instance of the Channels object. |
| <b>VB Syntax</b>   | <i>chans</i> .Resume                                                                                                                                                                                                    |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                             |
| <i>chans</i>       | A <a href="#">Channel collection</a> ( <b>object</b> )                                                                                                                                                                  |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                          |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                          |
| <b>Examples</b>    | <code>chans.Resume</code>                                                                                                                                                                                               |
| <b>C++ Syntax</b>  | HRESULT Resume();                                                                                                                                                                                                       |
| <b>Interface</b>   | IChannels2                                                                                                                                                                                                              |

Write-only

**Save Method**

---

**Description** Saves the appropriate content to the hard drive depending on the extension that is provided.

Some saved files can be recalled using `app.Recall`, depending on the content.

**VB Syntax** `app.Save(filename.ext)`

**Variable** **(Type) - Description**

`app` An Application (**object**)

`filename.ext` (**string**) - Full path, file name, and extension of the file.

Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents"  
Use one of the following extensions:

- **.cst** - Saves both Instrument State and Cal Set reference - Recalls a calibrated measurement. (Recallable)
- **.sta** - Saves Instrument State only - recalls the instrument state without calibration. (Recallable)
- **.cal** - Calibration file – saves the active Cal Sets currently in use by any channel. Use this mode for archival purposes only. All Cal Sets are saved to a Cal Set data file. This mode provides a method of safeguarding calibration data. This data can be restored to the list of Cal Sets available in the instrument. (Recallable)
- **.prn** - Saves active trace in comma-separated format (not recallable)
- **.bmp** - Saves a Bitmap of the screen (not recallable)
- **.s1p** - Saves 1-port measurement data (not recallable)
- **.s2p** - Saves 2-port measurement data (not recallable)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.Save("C:\Program Files\Agilent\Network Analyzer\Documents\Newfolder\MyState.cst) 'Saves "mystate.cst" to the specified folder`

**C++ Syntax** HRESULT Save(BSTR bstrFile)

**Interface** IApplication

## Save Method

---

**Description** Saves the current Cal Set to disk (recommended method for saving a Cal Set).

**Note:** There is also a Save method on the [ICalManager](#) and [Calibrator](#) interface which saves every Cal Set that currently exists in the instrument to the disk.

Learn more about [reading and writing Cal data using COM](#)

**VB Syntax** *CalSet.Save*

**Variable** **(Type) - Description**

*CalSet* **(object)** - A Cal Set object

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `myCalSet.Save`

See [Copy Method](#) for an example application of this command.

**C++ Syntax** HRESULT Save();

**Interface** ICalSet

## SaveCalSets Method

---

**Description** Writes new or changed Cal Sets out to disk. All Cal Sets are saved in a single file. This file is updated at the following times:

- When a Cal Set has been deleted.
- When a calibration has been performed through the front panel interface.
- When this method is called.
- When [ICalSet::Save](#) is called.

---

**Note:** The recommended method to save a Cal Set is [ICalSet::Save](#) which saves the data for **only** the current Cal Set to the disk. This method (ICalManager/Calibrator::SaveCalSets) saves **every** Cal Set that currently exists in the instrument to the disk.

---

Learn more about [reading and writing Cal data using COM](#)

**VB Syntax** *object*.SaveCalSets

**Variable** **(Type)** - Description

*object* **(object)** - A CalManager object or a Calibrator object

**Return Type** None

**Default** Not Applicable

**Example** `calMgr.SaveCalSets`

**C++ Syntax** HRESULT SaveCalSets( );

**Interface** ICalManager  
ICalibrator

Write-only

## SaveCitiDataData Method

---

**Description** Saves UNFORMATTED trace data to .cti file. [Learn more about citifiles.](#)

**VB Syntax** `app.SaveCitiDataData(filename.cti)`

**Variable** **(Type) - Description**

*app* An Application (**object**)

*filename.cti* **(string)** - Full path, file name, and .cti extension of the file.  
Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents".

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.SaveCitiDataData ("C:\Program Files\Agilent\Network Analyzer\Documents\myDDCitifile.cti") 'Saves "myDDCitifile.cti" to the specified folder`

**C++ Syntax** HRESULT SaveCitiDataData (BSTR bstrFile)

**Interface** IApplication5

## SaveCitiFormattedData Method

---

**Description** Saves FORMATTED trace data to .cti file. [Learn more about citifiles.](#)

**VB Syntax** `app.SaveCitiFormattedData(filename.cti)`

**Variable** **(Type) - Description**

*app* An [Application](#) (**object**)

*filename.cti* **(string)** - Full path, file name, and .cti extension of the file.  
Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents"

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.SaveCitiFormattedData ("C:\Program Files\Agilent\Network Analyzer\Documents\Newfolder\myFDCitifile.cti") 'Saves "myFDCitifile.cti" to the specified folder`

**C++ Syntax** HRESULT SaveCitiFormattedData (BSTR bstrFile)

**Interface** IApplication5



Write only

## SaveFile Method

---

**Description** Saves the mixer/converter test setup to a mixer attributes (.mxr) file.

**VB Syntax** *mixer*.**SaveFile** (*filename*)

**Variable** **(Type) - Description**

*mixer* An IMixer Interface pointer to a measurement **(object)**

*filename* (String) Full path, file name, and .mxr extension of the file.  
Files are typically stored in "C:\Program Files\Agilent\Network Analyzer\Documents".

**Return Type** String

**Default** Not Applicable

**Examples** `mixer.SaveFile ("C:\Program Files\Agilent\Network Analyzer\Documents\myMixer.mxr")`

**C++ Syntax** HRESULT put\_SaveFile(BSTR newVal)

**Interface** IMixer

Write-only

**SaveKits Method**

---

**Description** Saves the cal kits, typically after modifying a calibration kit. To load a cal kit into the analyzer from the hard drive, use [app.RecallKits](#).

**VB Syntax** `app.SaveKits`

**Variable** **(Type) - Description**

`app` An [Application](#) (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.SaveKits`

**C++ Syntax** `HRESULT SaveKits()`

**Interface** `IApplication`

## SearchFilterBandwidth Method

---

**Description** Searches the measurement data with the current [BandwidthTarget](#) (default is -3). To continually track the filter bandwidth, use [BandwidthTracking](#).

This feature uses markers 1-4. If not already, they are activated. To turn off these markers, either turn them off individually or [DeleteAllMarkers](#).

The bandwidth statistics are displayed on the analyzer screen. To get the bandwidth statistics, use either [GetFilterStatistics](#) or [FilterBW](#), [FilterCF](#), [FilterLoss](#), or [FilterQ](#).

The analyzer screen will show either Bandwidth statistics OR Trace statistics; not both.

To search a [UserRange](#) with the bandwidth search, first activate marker 1 and set the desired UserRange. Then send the SearchFilterBandwidth command. The user range used with bandwidth search only applies to marker 1 searching for the max value. The other markers may fall outside the user range.

**VB Syntax** `meas.SearchFilterBandwidth`

**Variable** **(Type) - Description**

`meas` A Measurement (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `meas.SearchFilterBandwidth`

**C++ Syntax** HRESULT SearchFilterBandwidth()

**Interface** IMeasurement

Write-only

## SearchMax Method

---

**Description** Searches the marker domain for the maximum value.

**VB Syntax** *mark*.SearchMax

**Variable** (Type) - Description

*mark* A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SearchMax`

**C++ Syntax** HRESULT SearchMax()

**Interface** IMarker

## SearchMin Method

---

**Description** Searches the marker domain for the minimum value.

**VB Syntax** *mark*.**SearchMin**

**Variable** (Type) - Description

*mark* A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SearchMin`

**C++ Syntax** HRESULT SearchMin()

**Interface** IMarker

Write-only

## SearchNextPeak Method

---

**Description** Searches the marker's domain for the next peak value.

**VB Syntax** *mark*.SearchNextPeak

**Variable** (Type) - Description

*mark* A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SearchNextPeak`

**C++ Syntax** HRESULT SearchNextPeak()

**Interface** IMarker

Write-only

## SearchPeakLeft Method

---

**Description** Searches the marker's domain for the next **VALID** peak to the left of the marker.

**VB Syntax** *mark*.SearchPeakLeft

**Variable** (Type) - Description

*mark* A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SearchPeakLeft`

**C++ Syntax** HRESULT SearchPeakLeft()

**Interface** IMarker

Write-only

## SearchPeakRight Method

---

**Description** Searches the marker's domain for the next **VALID** peak to the right of the marker.

**VB Syntax** *mark*.SearchPeakRight

**Variable** (Type) - Description

*mark* A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SearchPeakRight`

**C++ Syntax** HRESULT SearchPeakRight()

**Interface** IMarker



Write-only

**SearchTarget Method**

---

|                    |                                                                                                                                                                                                                 |
|--------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Searches the marker's domain for the target value (specified with <code>mark.TargetValue</code> ). Searches to the right; then at the end of the search domain, begins again at the start of the search domain. |
| <b>VB Syntax</b>   | <code>mark.SearchTarget</code>                                                                                                                                                                                  |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                     |
| <code>mark</code>  | A Marker ( <b>object</b> )                                                                                                                                                                                      |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                  |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                  |
| <b>Examples</b>    | <code>mark.SearchTarget</code>                                                                                                                                                                                  |
| <b>C++ Syntax</b>  | <code>HRESULT SearchTarget()</code>                                                                                                                                                                             |
| <b>Interface</b>   | IMarker                                                                                                                                                                                                         |

## SearchTargetLeft Method

---

**Description** Moving to the left of the marker position, searches the marker's domain for the target value (specified with [mark.TargetValue](#)).

**VB Syntax** *mark*.SearchTargetLeft

**Variable** **(Type) - Description**

*mark* A Marker **(object)**

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SearchTargetLeft`

**C++ Syntax** HRESULT SearchTargetLeft()

**Interface** IMarker

## SearchTargetRight Method

---

|                    |                                                                                                                                                   |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Moving to the right of the marker position, searches the marker's domain for the target value (specified with <a href="#">mark.TargetValue</a> ). |
| <b>VB Syntax</b>   | <i>mark</i> .SearchTargetRight                                                                                                                    |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                       |
| <i>mark</i>        | A Marker <b>(object)</b>                                                                                                                          |
| <b>Return Type</b> | Not Applicable                                                                                                                                    |
| <b>Default</b>     | Not Applicable                                                                                                                                    |
| <b>Examples</b>    | <code>mark.SearchTargetRight</code>                                                                                                               |
| <b>C++ Syntax</b>  | HRESULT SearchTargetRight()                                                                                                                       |
| <b>Interface</b>   | IMarker                                                                                                                                           |

**SelectCalSet Method**

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Selects a Cal Set to apply to the measurements on the calling channel.<br>If the cal set's GUID is not found, this method returns E_NA_Cal Set_NOT_FOUND.<br><b>Note:</b> Error Correction is not automatically applied as a result of this command being issued. If there is more than one Cal Type in the Cal Set, you must explicitly choose the Cal Type you want to apply. (See <a href="#">meas.CalType</a> )                                                                                                                          |
| <b>VB Syntax</b>   | <i>channel</i> . <b>SelectCalSet</b> <i>GUID</i> , <i>restore</i>                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <i>channel</i>     | <b>(object)</b> - A Channel object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <i>GUID</i>        | <b>(string)</b> - GUID number of the Cal Set to select                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <i>restore</i>     | <b>(boolean)</b> -<br><b>True (1)</b> - The stimulus stored with the cal set will be applied to the channel.<br><b>False (0)</b> - If a conflict is detected between the existing channel settings and the Cal Set stimulus settings, then the following will occur:<br>If interpolation is ON, then interpolation will be attempted. This may fail if the channel frequency is outside the range of the Cal Set.<br>If interpolation is OFF, the selection will be abandoned and an error is returned:<br>E_NA_CAL_STIMULUS_VALUES_EXCEEDED |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <b>Example</b>     | <code>channel.SelectCalSet GUID, 1</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
| <b>C++ Syntax</b>  | HRESULT SelectCalSet (BSTR strGUID, bool bRestore);                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <b>Interface</b>   | IChannel                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |

## SetAllSegments Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                  |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Uploads a segment table to the PNA replacing any existing segment table.<br>Segments must be ascending in frequency and non-overlapping. If they are not, the segments are 'adjusted' as they are from the front panel control. The total number of points for all segments cannot exceed the PNA maximum for a sweep.<br><a href="#">See an example</a> that uses this command. |
| <b>VB Syntax</b>   | <i>Segs</i> . <b>SetAllSegments</b> ( <i>segdata</i> )                                                                                                                                                                                                                                                                                                                           |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                      |
| <i>segs</i>        | A Segments ( <b>Collections</b> )                                                                                                                                                                                                                                                                                                                                                |
| <i>segdata</i>     | Variant or Double Array - Segment data<br>For VARIANT, the underlying type must be appropriate for the element:<br>Boolean - segment on/off<br>Integer - number of points<br>Double - all other elements.                                                                                                                                                                        |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                   |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                   |
| <b>Examples</b>    | <a href="#">See an example using this command</a>                                                                                                                                                                                                                                                                                                                                |
| <b>C++ Syntax</b>  | SetAllSegments (VARIANT Segments );                                                                                                                                                                                                                                                                                                                                              |
| <b>Interface</b>   | ISegments2                                                                                                                                                                                                                                                                                                                                                                       |

**SetBBPorts Method**

**Description** For a Balanced - Balanced device type, maps the PNA ports to the DUT ports.


Set the Balanced device type using the [DUTTopology Property](#)

**VB Syntax** *balTopology*.**SetBBPorts** *p1Pos, p1Neg, p2Pos, p2Neg*

**Variable** **(Type) - Description**

*balTopology* A [BalancedTopology](#) (**object**)

*p1Pos, p1Neg, p2Pos, p2Neg* (**Long Integer**) PNA port number that connects to each of the following DUT ports:

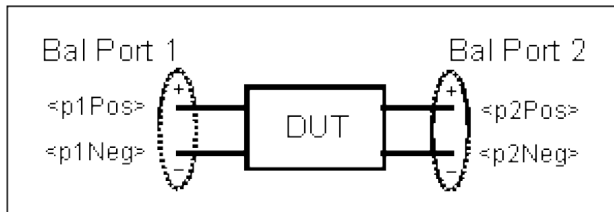

**Return Type** Not applicable - To read port mappings, use the [BalancedTopology](#) properties.

**Default** Not Applicable

**Examples** `balTop.SetBBPorts 1,2,3,4`

**C++ Syntax** HRESULT SetBBPorts (long p1Pos, long p1Neg, long p2Pos, long p2Neg)

**Interface** IBalancedTopology

**SetCallInfo Method**

---

**Description** Specifies the type of calibration. This method should be the first method called on the calibrator object. It prepares the internal state for the rest of the calibration.

**Note:** You can NOT perform a 3 or 4-port cal using SetCallInfo even though there is enumCalTypes. You must use the [GuidedCalibration](#) object.

Learn more about [reading and writing Cal data using COM](#)

The analyzer can measure both ports simultaneously, assuming you have two of each standard type. For a 2-port cal, See [cal.Simultaneous2PortAcquisition](#)

**VB Syntax** *cal.SetCallInfo (type,rcvPort,srcPort)*

**Variable** **(Type) - Description**

*cal* A Calibrator **(object)**

*type* **(enum NACalType)** - Calibration type. Choose from:

- 0 - naCalType\_Response\_Open
- 1 - naCalType\_Response\_Short
- 2 - naCalType\_Response\_Thru
- 3 - naCalType\_Response\_Thru\_And\_Isol
- 4 - naCalType\_OnePort
- 5 - naCalType\_TwoPort\_SOLT
- 6 - naCalType\_TwoPort\_TRL
- 7 - naCalType\_None
- 8 - naCalType\_ThreePort\_SOLT
- 9 - Custom
- 10 - naCalType\_FourPort\_SOLT

**Note:** For 1-port cals, the source port = receiver port. For 2, 3,4-port SOLT and TRL, it doesn't matter which port is specified as source and receiver

*rcvPort* **(long integer)** - Receiver Port

*srcPort* **(long integer)** - Source Port

**Return Type** NACalType

**Default** 7-naCalType\_None

**Examples** `cal.setCalInfo(naCalType_Response_Open,1,1)`

**C++ Syntax** HRESULT SetCallInfo(tagNACalType calType,long portA, long portB)

**Interface** ICalibrator





**SetCalInfo2 Method (for source power cal)**

|                        |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
|------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b>     | Specifies the technique, the channel, and the source port to be used for the source power calibration about to be performed.                                                                                                                                                                                                                                                                                                                                                                                          |
|                        | <b>Note:</b> This method replaces <u>SetCalInfo Method</u> .                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <b>VB Syntax</b>       | <code>powerCalibrator.<b>SetCalInfo2</b> calMethod, channel, sourcePort, [powerOffset,] [display]</code>                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Variable</b>        | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <i>powerCalibrator</i> | <b>(object)</b> - A <u>SourcePowerCalibrator3</u> object                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <i>calMethod</i>       | <b>(enum NASourcePowerCalMethod)</b> Selects the calibration method to be used for the source power cal acquisition.<br><br><b>0 – naPowerMeter</b> Power Meter is used for all readings. (same as " <u>fast iteration</u> " box not checked on dialog box)<br><br><b>1 - naPowerMeterAndReceiver</b> Power meter for the first iteration; then use the reference receiver for remaining readings if necessary (same as " <u>fast iteration</u> " box checked on dialog box)                                          |
| <i>channel</i>         | <b>(long integer)</b> - Number of the PNA channel (not power meter channel) on which the source power cal will be performed. If the channel does not already exist, it will be created.                                                                                                                                                                                                                                                                                                                               |
| <i>sourcePort</i>      | <b>(long integer)</b> - Port number on which the source power cal will be performed.                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <i>[powerOffset]</i>   | <b>(double)</b> - Optional argument. Sets or returns a power level offset from the PNA test port power. This can be a gain or loss value (in dB) to account for components you connect between the source and the reference plane of your measurement. For example, specify 10 dB to account for a 10 dB amplifier at the input of your DUT. Following the calibration, the PNA power readouts are adjusted by this value. This argument performs the same function as <u>chan.SourcePowerCalPowerOffset Property</u> |
| <i>[display]</i>       | <b>(boolean)</b> Optional argument. Enables and disables the display of power readings on the PNA screen. After the source power cal data is acquired, this setting is reset to ON. If unspecified, value is set to ON.<br><br><b>True</b> - Display of power readings is ON<br><b>False</b> - Display of power readings is OFF                                                                                                                                                                                       |
| <b>Return Type</b>     | None                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| <b>Default</b>         | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| <b>Examples</b>        | <code>powerCalibrator.SetCalInfo2 naPowerMeter, 1, 1, -10, True</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>C++ Syntax</b>      | <code>HRESULT SetCalInfo2( tagNASourcePowerCalMethod enumCalMethod, long Channel, long SourcePort, double PowerOffset = 0., VARIANT_BOOL bDisplay = VARIANT_TRUE);</code>                                                                                                                                                                                                                                                                                                                                             |
| <b>Interface</b>       | ISourcePowerCalibrator3                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |



## SetCenter Method

---

|                    |                                                                                                                                                                                                                                  |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Changes the center stimulus to the stimulus value of the marker. The start stimulus stays the same and the stop is adjusted.<br><br>This command does not work with channels that are in <u>CW</u> or <u>Segment Sweep</u> mode. |
| <b>VB Syntax</b>   | <i>mark</i> .SetCenter                                                                                                                                                                                                           |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                      |
|                    | <i>mark</i> A Marker <b>(object)</b>                                                                                                                                                                                             |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                   |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                   |
| <b>Examples</b>    | <code>mark.SetCenter</code>                                                                                                                                                                                                      |
| <b>C++ Syntax</b>  | HRESULT SetCenter()                                                                                                                                                                                                              |
| <b>Interface</b>   | IMarker                                                                                                                                                                                                                          |

## SetCW Method

---

|                    |                                                                                                                                                                                 |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Changes the analyzer to sweep type CW mode and sets the CW frequency to the marker's frequency. Does not change anything if current sweep type is other than a frequency sweep. |
| <b>VB Syntax</b>   | <i>mark</i> .SetCW                                                                                                                                                              |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                     |
| <i>mark</i>        | A Marker <b>(object)</b>                                                                                                                                                        |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                  |
| <b>Default</b>     | Not Applicable                                                                                                                                                                  |
| <b>Examples</b>    | <code>mark.SetCW</code>                                                                                                                                                         |
| <b>C++ Syntax</b>  | HRESULT SetCW()                                                                                                                                                                 |
| <b>Interface</b>   | IMarker                                                                                                                                                                         |

## SetElectricalDelay Method

---

**Description** Changes the measurement's electrical delay to the marker's delay value.

**VB Syntax** *mark*.SetElectricalDelay

**Variable** (Type) - Description

*mark* A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SetElectricalDelay`

**C++ Syntax** HRESULT SetElectricalDelay()

**Interface** IMarker

## SetFailOnOverRange Method

---

**Description** When set TRUE, configures the analyzer to report outOfRange conditions with an **error** code. Any overrange error will return **E\_NA\_LIMIT\_OUTOFRANGE\_ERROR**.

**Note:** This method is for the benefit of VB clients. The analyzer automatically adjusts overrange conditions to the closest acceptable setting. The VB user will not see that an overrange occurred because the HRESULT is not returned if it has a success code. For more information, see [Events/OverRange](#).

**VB Syntax** `app.SetFailOnOverRange state`

**Variable** **(Type) - Description**

`app` An [Application](#) (**object**)

`state` (**boolean**) -  
**True (1)** - Overrange conditions report an error code  
**False (0)** - Overrange conditions report a success code

**Return Type** Not Applicable

**Default** False (0)

**VB Example**

```
app.SetFailOnOverRange TRUE
On Error Goto ERRHANDLER

'the following overrange will cause ERRHANDLER to be invoked

channel.StartFrequency = 9.9 GHZ
exit

ERRHANDLER:
 print "something failed"
```

**C++ Syntax** HRESULT put\_SetFailOnOverRange(VARIANT\_BOOL mode)

**Interface** IApplication

## SetPowerAcquisitionDevice Method

---

**Description** Sets the power sensor channel (A or B) to be used. This performs the same function as the **Use this sensor only** checkbox in the [Power Sensor Settings](#) dialog.

**Note:** This method is only necessary when performing an SMC calibration.

---

**VB Syntax** `pwrCal.SetPowerAcquisitionDevice sensor`

**Variable** **(Type) - Description**

`pwrCal` (Object) A [SourcePowerCalibrator](#) object

`sensor` (**enum NAPowerAcquisitionDevice**) The power sensor channel. Choose from:

0 – naPowerSensor\_A

1 – naPowerSensor\_B

**Default** Not Applicable

**Examples** `pwrCal.PowerAcquisitionDevice naPowerSensor_A`

**C++ Syntax** HRESULT SetPowerAcquisitionDevice( tagNAPowerAcquisitionDevice enumAcqDevice);

**Interface** ISourcePowerCalibrator3

Write-only

**SetFrequencyLowPass Method**

---

**Description** Set the start frequencies when **trans.Mode = LowPass**.**VB Syntax** *trans*.**SetFrequencyLowPass****Variable** (Type) - Description*trans* A Transform (**object**)**Return Type** Not Applicable**Default** Not Applicable**Examples** `trans.SetFrequencyLowPass`**C++ Syntax** HRESULT SetFrequencyLowPass(void)**Interface** ITransform



## SetReferenceLevel Method

---

**Description** Changes the measurement's reference level to the marker's Y-axis value.

**VB Syntax** *mark*.SetReferenceLevel

**Variable** (Type) - Description

*mark* A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SetReferenceLevel`

**C++ Syntax** HRESULT SetReferenceLevel()

**Interface** IMarker

**SetSBPorts Method**

---


**Description** For a Single-ended - Balanced device type, maps the PNA ports to the DUT ports.  
Set the Single-ended - Balanced device type using the [DUTTopology Property](#)

**VB Syntax** *balTopology.SetSBPorts se, bPos, bNeg*

**Variable** **(Type) - Description**

*balTopology* A [BalancedTopology](#) (**object**)

*se, bPos, bNeg* PNA port number that connects to each of the following DUT ports:

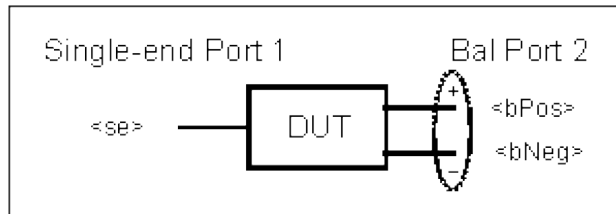

**Return Type** Not applicable - To read port mappings, use the [BalancedTopology](#) properties.

**Default** Not Applicable

**Examples** `balTop.SetSBPorts 1,2,3`

**C++ Syntax** HRESULT SetSBPorts (long se, long bPos, long bNeg)

**Interface** IBalancedTopology

## SetSSBPorts Method

---

**Description** For a Single-ended - Single-ended - Balanced device type, maps the PNA ports to the DUT ports.


Set the Single-ended - Single-ended - Balanced device type using the [DUTTopology Property](#)

**VB Syntax** `balTopology.SetSSBPorts se, se2, bPos, bNeg`

**Variable (Type) - Description**

`balTopology` A [BalancedTopology \(object\)](#)

`se, se2, bPos, bNeg` PNA port number that connects to each of the following DUT ports:

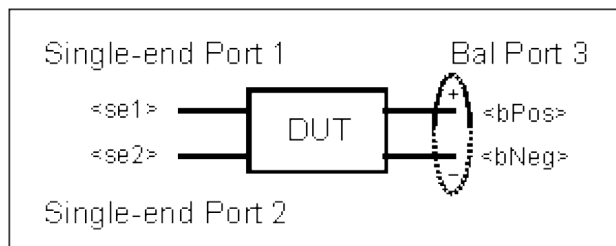

**Return Type** Not applicable - To read port mappings, use the [BalancedTopology](#) properties.

**Default** Not Applicable

**Examples** `balTop.SetSSBPorts 1,2,3,4`

**C++ Syntax** HRESULT SetSSBPorts (long se, long se2, long bPos, long bNeg)

**Interface** IBalancedTopology

Write-only

## SetStandardsForClass Method

---

**Description** Set the calibration standard numbers for a specified calibration class. To read the cal standard numbers use [GetStandardsForClass Method](#)

**VB Syntax** `calKit.SetStandardsForClass (calclassorder, std1, std2, std3, std4, std5, std6, std7)`

**Variable** **(Type) - Description**

`calKit` A CalKit (**object**)

`calclassorder` (**enum NACalClassOrder**) Cal Class. Choose from:

0 - naRefl\_1\_S11

1 - naRefl\_2\_S11

2 - naRefl\_3\_S11

3 - naTran\_1\_S21

4 - naRefl\_1\_S22

5 - naRefl\_2\_S22

6 - naRefl\_3\_S22

7 - naTran\_1\_S12

8 - naRefl\_1\_S33

9 - naRefl\_2\_S33

10 - naRefl\_3\_S33

11 - naTran\_1\_S32

12 - naTran\_1\_S23

13 - naTran\_1\_S31

14 - naTran\_1\_S13

15 - naTRL\_T

16 - naTRL\_R

17 - naTRL\_L

`std1...std7` (**long**) Calibration Standard Number. Choose from **1** through **30**. Std2 through Std7 are optional

**Return Type** Not applicable

**Default** Not applicable

**Examples** `calkit.SetStandardsForClass naRefl_3_S11, 3, 5, 6`  
`calkit.SetStandardsForClass naTran_1_S21, 4`

**C++ Syntax** HRESULT SetStandardsForClass(NACalClassOrder calclassorder, long std1, long std2, long std3, long std4, long std5, long std6, long std7)

**Interface** ICalkit

## SetStart Method

---

**Description** Changes the start stimulus to the stimulus value of the marker. The stop stimulus stays the same and the span is adjusted.

This command does not work with channels that are in [CW](#) or [Segment Sweep](#) mode.

**VB Syntax** `mark.SetStart`

**Variable** **(Type) - Description**

`mark` A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SetStart`

**C++ Syntax** HRESULT SetStart()

**Interface** IMarker

## SetStop Method

---

**Description** Changes the stop stimulus to the stimulus value of the marker. The start stimulus stays the same and the span is adjusted.

This command does not work with channels that are in [CW](#) or [Segment Sweep](#) mode.

**VB Syntax** `mark.SetStop`

**Variable** **(Type) - Description**

`mark` A Marker (**object**)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `mark.SetStop`

**C++ Syntax** `HRESULT SetStop()`

**Interface** `IMarker`

## ShowMarkerReadout Method

---

|                    |                                                                                                               |
|--------------------|---------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Shows and Hides the Marker readout for the active marker in the upper-right corner of the window.             |
| <b>VB Syntax</b>   | <i>win</i> . <b>ShowMarkerReadout</b> <i>state</i>                                                            |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                   |
| <i>win</i>         | A NAWindow <b>(object)</b>                                                                                    |
| <i>state</i>       | <b>(boolean) -</b><br><b>True (1)</b> - Show the Marker readout<br><b>False (0)</b> - Hide the Marker readout |
| <b>Return Type</b> | Not Applicable                                                                                                |
| <b>Default</b>     | Not Applicable                                                                                                |
| <b>Examples</b>    | <code>win.ShowMarkerReadout True</code>                                                                       |
| <b>C++ Syntax</b>  | HRESULT ShowMarkerReadout(VARIANT_BOOL bState)                                                                |
| <b>Interface</b>   | INAWindow                                                                                                     |



## ShowStatusBar Method

---

**Description** Shows and Hides the Status Bar. The Status Bar is located across the bottom of the display. The following information is shown for the active measurement:

- Channel number
- Parameter
- Correction On or Off
- Remote or Local operation

**VB Syntax** `app.ShowStatusBar state`

**Variable** (Type) - Description

*app* An Application (**object**)

*state* (**boolean**) -  
**True (1)** - Show the Status Bar  
**False (0)** - Hide the Status Bar

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.ShowStatusBar True`

**C++ Syntax** HRESULT ShowStatusBar (VARIANT\_BOOL bState)

**Interface** IApplication

## ShowStimulus Method

---

|                    |                                                                                                                                                                  |
|--------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Shows and Hides the Stimulus (X-axis) information located at the bottom of the display. The start and stop stimulus values are shown for the active measurement. |
| <b>VB Syntax</b>   | <i>app</i> . <b>ShowStimulus</b> <i>state</i>                                                                                                                    |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                      |
| <i>app</i>         | An <u>Application</u> ( <b>object</b> )                                                                                                                          |
| <i>state</i>       | <b>(boolean) -</b><br><b>True (1)</b> - Show the Stimulus information<br><b>False (0)</b> - Hide the Stimulus information                                        |
| <b>Return Type</b> | Not Applicable                                                                                                                                                   |
| <b>Default</b>     | Not Applicable                                                                                                                                                   |
| <b>Examples</b>    | <code>app.ShowStimulus True</code>                                                                                                                               |
| <b>C++ Syntax</b>  | HRESULT ShowStimulus(VARIANT_BOOL bState)                                                                                                                        |
| <b>Interface</b>   | IApplication                                                                                                                                                     |

**ShowTable Method**

---

**Description** Shows or Hides the specified table for the window's active measurement in the lower part of the window.

**VB Syntax** *win.ShowTable value*

**Variable** **(Type) - Description**

*win* A NAWindow **(object)**

*value* **(enum naTable)** - The table to show or hide. Choose from:

0 - naTable\_None

1 - naTable\_Marker

2 - naTable\_Segment

3 - naTable\_Limit

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `win.ShowTable naTable_limit`

**C++ Syntax** HRESULT ShowTable (tagNATableType table)

**Interface** INAWindow

## ShowTitleBars Method

---

**Description** Shows and Hides the Title Bars. The Title Bars are across the top of the Network Analyzer Window and each of the measurement windows. The Window name is shown in the Title Bar.

**VB Syntax** `app.ShowTitleBars state`

**Variable** **(Type) - Description**

*app* An Application (**object**)

*state* (**boolean**)  
**True (1)** - Show the Title Bars  
**False (0)** - Hide the Title Bars

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `app.ShowTitleBars True`

**C++ Syntax** HRESULT ShowTitleBars\(\VARIANT\_BOOL bState)

**Interface** IApplication

## ShowToolbar Method

---

**Description** Shows and Hides the specified Toolbar.

**VB Syntax** `app.ShowToolbar toolbar,state`

**Variable** **(Type) - Description**

*app* An [Application](#) (**object**)

*toolbar* **(enum NAToolbarType)** - The toolbar to show or hide. Choose from:

- 0 - naToolbar\_None
- 1 - naToolbar\_ActiveEntry
- 2 - naToolbar\_Markers
- 3 - naToolbar\_Measurement
- 4 - naToolbar\_Stimulus
- 5 - naToolbar\_SweepControl

*state* **(boolean)** -  
**True (1)** - Show the specified toolbar  
**False (0)** - Hide the specified toolbar

**Return Type** Not Applicable

**Default** 1 - naToolbar\_ActiveEntry showing; all others hiding.

**Examples** `app.ShowToolbar 1,1 'shows the active entry toolbar`

**C++ Syntax** HRESULT ShowToolbar(tagNAToolbarType toolbar, VARIANT\_BOOL bState)

**Interface** IApplication

Write-only

## Single Method

---

**Description** Sets the trigger count to 1, which will cause the channel to respond to exactly one trigger signal from any source (internal, external, or manual).

**VB Syntax** `chan.Single [sync]`

**Variable** **(Type) - Description**

`chan` A Channel **(object)**

`[sync]` **(boolean)** -Optional argument. A variable set to either True or False.

**True** - The analyzer waits until the trigger is completed to process subsequent commands.

**False** - Subsequent commands are processed immediately.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
sync = True
chan.Single sync
```

**C++ Syntax** HRESULT Single(VARIANT\_BOOL bWait)

**Interface** IChannel

## StringToNACalClass Method

---

**Description** Converts the returned strings from [GetStandardsList](#) into the enumeration (NACalClass) and the port numbers required for [PutStandard](#) and [GetStandard](#) methods that transmit data in and out of the Cal Set.

Learn more about [reading and writing Cal data using COM](#)

**VB Syntax** *CalSet*.**StringToNACalClass** (*list, std, rcv, src*)

**Variable** **(Type) - Description**

*CalSet* **(object)** - A Cal Set object

*list* **(string)** - a string containing the textual description of the standard.

*std* **(enum NACalClass)** Choose from:

1 - naClassA

2 - naClassB

3 - naClassC

4 - naClassD

5 - naClassE

6 - naReferenceRatioLine

7 - naReferenceRatioThru

### SOLT Standards

1 - naSOLT\_Open

2 - naSOLT\_Short

3 - naSOLT\_Load

4 - naSOLT\_Thru

5 - naSOLT\_Isolation

### TRL Standards

1 - naTRL\_Reflection

2 - naTRL\_Line\_Reflection

3 - naTRL\_Line\_Tracking

4 - naTRL\_Thru

5 - naTRL\_Isolation

*rcv* **(long)** - port number of the receiver

*src* **(long)** - port number of the source

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `guid = CalSet.StringToNACalClass(list, std, rcv, src)`

**C++ Syntax** HRESULT StringtoNACalClass ( BSTR\* str, NACalClass\* item, long \*rcv, long \*src);

**Interface** ICalSet



## StringToNAErrorTerm2 Method

---

**Description** Converts the returned strings from [GetErrorTermList](#) into the enumeration (NAErrorTerm2) and the port numbers required for [PutErrorTerm](#) and [GetErrorTerm](#) methods that transmit data in and out of the Cal Set.

Learn more about [reading and writing Cal data using COM](#)

**VB Syntax** *Cal Set*.StringToNAErrorTerm2 (*list, eterm, rcv, src*)

**Variable** [\(Type\)](#) - Description

*Cal Set* **(object)** - A Cal Set object

*list* **(string)** - a string containing the textual description of the error term.

*eterm* **(enum As NaErrorTerm2)**. Choose from:

- 0 - naET\_Directivity (rcv = src)
- 1 - naET\_SourceMatch (rcv = src)
- 2 - naET\_ReflectionTracking (rcv = src)
- 3 - naET\_TransmissionTracking (rcv != src)
- 4 - naET\_LoadMatch (rcv != src)
- 5 - naET\_Isolation (rcv != src)

*rcv* **(long)** - port number of the receiver

*src* **(long)** - port number of the source

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `CalSet.StringToNAErrorTerm2 str, term, rcv, src`

**C++ Syntax** HRESULT StringToNAErrorTerm2 (BSTR\* str, NAErrorTerm2\* item, long \*rcv, long \*src);

**Interface** ICalSet

## UserPreset Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                             |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Performs a User Preset. There must be an active User Preset state file (see <a href="#">UserPresetLoadFile</a> and <a href="#">UserPresetSaveState</a> ) or an error will be returned.<br><br>Regardless of the state of the <a href="#">User Preset Enable</a> checkbox, the <code>app.Preset</code> command will always preset the PNA to the factory preset settings, and <code>app.UserPreset</code> will always perform a User Preset. |
| <b>VB Syntax</b>   | <code>app.UserPreset</code>                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                 |
|                    | <code>app</code> An <a href="#">Application</a> ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Examples</b>    | <code>app.UserPreset</code>                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <b>C++ Syntax</b>  | <code>HRESULT UserPreset()</code>                                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Interface</b>   | <code>IApplication6</code>                                                                                                                                                                                                                                                                                                                                                                                                                  |

## UserPresetLoadFile Method

---

- Description** Loads an existing instrument state file (.sta or .cst) to be used for User Preset. Subsequent execution of app.UserPreset will cause the PNA to assume this instrument state.
- Regardless of the state of the User Preset Enable checkbox, the app.Preset command will always preset the PNA to the factory preset settings, and app.UserPreset will always perform a User Preset.
- VB Syntax** `app.UserPresetLoadFile (file)`
- Variable** **(Type) - Description**
- `app` An Application (**object**)
- `file` (**String**) Full path, name, and extension of the file to be loaded.
- Return Type** Not Applicable
- Default** Not Applicable
- Examples** `app.UserPresetLoadFile ("C:\Program Files\Agilent\Network Analyzer\Documents\10MHzto20GHz.sta")`
- C++ Syntax** HRESULT UserPresetLoadFile (BSTR bstrFile)
- Interface** IApplication6

## UserPresetSaveState Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | Saves the current instrument settings as UserPreset.sta. Subsequent execution of <a href="#">app.UserPreset</a> will cause the PNA to assume this instrument state.<br><br>Regardless of the state of the <a href="#">User Preset Enable</a> checkbox, the <a href="#">app.Preset</a> command will always preset the PNA to the factory preset settings, and <a href="#">app.UserPreset</a> will always perform a User Preset. |
| <b>VB Syntax</b>   | <code>app.UserPresetSaveState</code>                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                    |
|                    | <code>app</code> An <a href="#">Application</a> ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                                              |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Examples</b>    | <code>app.UserPresetSaveState</code>                                                                                                                                                                                                                                                                                                                                                                                           |
| <b>C++ Syntax</b>  | <code>HRESULT UserPresetSaveState()</code>                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>Interface</b>   | <code>IApplication6</code>                                                                                                                                                                                                                                                                                                                                                                                                     |

**WriteData Method**

---

- Description** Writes a 13-bit value to the specified address using the AD0 through AD12 lines of the external test set connector. The PNA generates the appropriate timing signals. It automatically controls timing signals LDS, LAS and RLW to strobe the address, then the data, to the external test set. See the [timing diagram](#) for Address and Data I/O read.
- VB Syntax** *ExtIO.WriteData (address) = value*
- Variable (Type) - Description**
- ExtIO* **(object)** - An [External IO object](#)
- address* **(variant)** - Address to be written to.
- value* **(variant)** - 13-bit word to write
- Return Type** Not Applicable
- Default** Not Applicable
- Examples** `ExtIO.WriteData (15) = 12`
- C++ Syntax** HRESULT WriteData(VARIANT Address, VARIANT Data);
- Interface** IHWExternalTestSetIO

**WriteRaw Method**

**Description** Writes a 16-bit value to the external test set connector lines AD0 - AD12, RLW, LAS and LDS. The analyzer does NOT generate the appropriate timing signals. The user has control of all 16 lines using this write method.

**Note:** When RLW (pin25) is set to 1 (high) it causes lines AD0 - AD12 to float. It disables their output latches and sets the hardware for reading. LDS and LAS are not affected by this behavior.

**Below is the format of data that is written with WriteRaw:**

\* This Output will float if RLW (bit-13) is set high

| Pin | Bit | Signal name |
|-----|-----|-------------|
| 22  | 0   | AD0*        |
| 23  | 1   | AD1*        |
| 11  | 2   | AD2*        |
| 10  | 3   | AD3*        |
| 9   | 4   | AD4*        |
| 21  | 5   | AD5*        |
| 20  | 6   | AD6*        |
| 19  | 7   | AD7*        |
| 6   | 8   | AD8*        |
| 5   | 9   | AD9*        |
| 4   | 10  | AD10*       |
| 17  | 11  | AD11*       |
| 3   | 12  | AD12*       |
| 25  | 13  | RLW         |
| 24  | 14  | LDS         |
| 8   | 15  | LAS         |

**VB Syntax** *ExtIO.WriteRaw* *value*

**Variable** **(Type) - Description**

*ExtIO* **(object)** - An External IO object

*value* **(variant)** - Data to be written

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `ExtIO.WriteRaw 12`

**C++ Syntax** HRESULT WriteRaw( VARIANT Output );

**Interface** IHWExternalTestSetIO

## OnCalEvent

---

**Description** Triggered by a calibration event. See a list of [CAL Events](#).

**Note:** Some Severe Events are also used as Error Messages

---

**VB Syntax** Sub *app*\_**OnCalEvent**(ByVal *eventID* As Variant, ByVal *chanNum* As Variant, ByVal *measNum* As Variant)

**Variable** **(Type) - Description**

*app* An Application (**object**)

*eventID* Code number of the event which occurred

*chanNum* Channel Number of the event

*measNum* Measurement Number of the event

**Return Type** Not Applicable

**Default** Not Applicable

**Examples**

```
Sub pna_OnCalEvent(ByVal eventID As Variant, ByVal
channelNumber As Variant, ByVal measurementNumber As Variant)
'
MsgBox ("A Calibration event has occurred")
End Sub
```

---

**C++ Syntax** HRESULT OnCalEvent(VARIANT eventID, VARIANT channelNumber, VARIANT measurementNumber)

**Interface** IApplication



## OnChannelEvent

---

**Description** Triggered by a channel event. See a list of [Channel Events](#)

---

**Note:** Some Severe Events are also used as Error Messages

---

**VB Syntax** Sub *app\_OnChannelEvent*(ByVal *eventID* As Variant, ByVal *chanNum* As Variant)

---

**Variable** **(Type) - Description**

*app* An Application (**object**)

*eventID* Code number of the event which occurred

*chanNum* Channel Number of the event

**Return Type** Not Applicable

**Default** Not Applicable

---

**Examples**

```
Sub pna_OnChannelEvent(ByVal eventID As Variant, ByVal
channelNumber As Variant)
 MsgBox "A channel event occurred"
End Sub
```

---

**C++ Syntax** HRESULT OnChannelEvent(VARIANT eventID, VARIANT channelNumber)

**Interface** IApplication

## OnDisplayEvent

---

**Description** Triggered by a display event. See a list of [Display Events](#)

**Note:** Some Severe Events are also used as Error Messages

---

**VB Syntax** Sub *app*\_**OnDisplayEvent**(ByVal *eventID* As Variant, ByVal *winNum* As Variant, ByVal *traceNum* As Variant)

---

**Variable** **(Type) - Description**

*app* An Application (**object**)

*eventID* Code number of the event which occurred

*winNum* Window Number of the event

*traceNum* Trace Number of the event

**Return Type** Not Applicable

**Default** Not Applicable

---

**Examples**

```
Sub pna_OnDisplayEvent(ByVal eventID As Variant, ByVal
windowNumber As Variant, ByVal traceNumber As Variant)
MsgBox ("A Display event has occurred")
End Sub
```

---

**C++ Syntax** HRESULT OnDisplayEvent(VARIANT eventID, VARIANT windowNumber, VARIANT traceNumber)

**Interface** IApplication

## OnHardwareEvent

---

**Description** Triggered by a hardware event. See a list of [Hardware Events](#)

**Note:** Some Severe Events are also used as Error Messages

---

**VB Syntax** Sub *app*\_**OnHardwareEvent**(ByVal *eventID* As Variant)

---

**Variable** (Type) - Description

*app* An Application (**object**)

*eventID* Code number of the event which occurred

**Return Type** Not Applicable

**Default** Not Applicable

---

**Examples**

```
Private Sub pna_OnHardwareEvent(ByVal eventID As Variant)
 MsgBox ("A Hardware event has occurred")
End Sub
```

---

**C++ Syntax** HRESULT OnHardwareEvent(VARIANT eventID)

**Interface** IApplication

## OnMeasurementEvent

---

**Description** Triggered by a measurement event. See a list of [Measurement Events](#).

**Note:** Some Severe Events are also used as Error Messages

---

**VB Syntax** Sub *app\_OnMeasurementEvent*(ByVal *eventID* As Variant, ByVal *measNum* As Variant)

---

**Variable** **(Type) - Description**

*app* An Application (**object**)

*eventID* Code number of the event which occurred

*measNum* Measurement Number of the event

**Return Type** Not Applicable

**Default** Not Applicable

---

**Examples**

```
Private Sub pna_OnMeasurementEvent(ByVal eventID As Variant, ByVal
measurementNumber As Variant)

MsgBox ("A Measurement event has occurred")

End Sub
```

---

**C++ Syntax** HRESULT OnMeasurementEvent(VARIANT eventID, VARIANT measurementNumber)

**Interface** IApplication

## OnSCPIEvent

---

**Description** Triggered by a SCPI event. See a list of [SCPI Events](#)

**Note:** Some Severe Events are also used as Error Messages

---

**VB Syntax** Sub *app*\_**OnSCPIEvent**(ByVal *eventID* As Variant)

---

**Variable** (Type) - Description

*app* An Application (**object**)

*eventID* Code number of the event which occurred

**Return Type** Not Applicable

**Default** Not Applicable

---

**Examples**

```
Private Sub pna_OnSCPIEvent(ByVal eventID As Variant)
 MsgBox ("A SCPI event has occurred")
End Sub
```

---

**C++ Syntax** HRESULT OnSCPIEvent(VARIANT eventID )

**Interface** IApplication

## OnSystemEvent

---

**Description** Triggered by a system event. See a list of [System Events](#), also known as general events.

**Note:** Some Severe Events are also used as Error Messages

---

**VB Syntax** Sub *app\_OnSystemEvent*(ByVal *eventID* As Variant)

---

**Variable** **(Type) - Description**

*app* An Application (**object**)

*eventID* Code number of the event which occurred

*chanNum* Channel Number of the event

**Return Type** Not Applicable

**Default** Not Applicable

---

**Examples**

```
Private Sub pna_OnSystemEvent(ByVal eventID As Variant)
 MsgBox ("A System event has occurred")
End Sub
```

---

**C++ Syntax** HRESULT OnSystemEvent(VARIANT eventID)

**Interface** IApplication

## OnUserEvent

---

**Description** Reserved for future use.

**VB Syntax** Sub app\_**OnUserEvent**

## Reading Cal Set Data using COM

---

This example iterates over the entire collection of Cal Sets that currently reside in the PNA. It reads the entire list of error term strings from each Cal Set and queries the data for each term. It then does the same for the standards data.

Learn more about [Reading and Writing Calibration data using COM](#).

Learn more about [Cal Sets](#).

### See Other COM Example Programs

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save on the PNA hard drive as CalSets.vbs. [Learn how to setup and run the macro](#).

```
Dim pna
Dim cset
Dim calsets

' create the pna object
' to run on a remote PC, substitute 'name' for the full computer name of your PNA
' to run as a macro on the PNA, remove , "name"
Set pna = CreateObject("AgilentPNA835x.Application", "name")
wscript.echo pna.IDString
' obtain the calset collection
Set calsets = pna.GetCalManager.calsets

' loop thru the calsets
Dim c
For c = 1 To calsets.count
Set cset = calsets.Item(c)

' wscript.echo prints values to a message box
wscript.echo "calset = ", cset.GetGUID, cset.Description

' iterate through error terms data
Dim vterms
vterms = cset.GetErrorTermList2(0, "")
if (Not IsEmpty(vterms)) then
For i = LBound(vterms) To UBound(vterms)
wscript.echo vterms(i)
vdata = cset.GetErrorTermByString(0,vterms(i))
wscript.echo vdata(1,0), vdata(1,1)
Next
end if

' iterate through standards data
vterms = cset.GetStandardList2("")
if (Not IsEmpty(vterms)) then
For i = LBound(vterms) To UBound(vterms)
wscript.echo vterms(i)
vdata = cset.GetStandardByString(vterms(i))
wscript.echo vdata(1,0), vdata(1,1)
Next
```



```
end if
Next
```

## Getting Trace Data from the Analyzer

---

This Visual Basic program:

- Retrieves Scalar Data from the Analyzer and plots it.
- Retrieves Paired Data from the Analyzer and plots it.
- Retrieves Complex Data from the Analyzer and plots it.

To use this code, prepare a form with the following:

- Two MSCharts named **MSChart1** and **MSChart2**
- Three buttons named **GetScalar**, **GetPaired**, **GetComplex**

---

**Note:** You can get MSChart in Visual Basic by clicking **Project / Components / Microsoft Chart Control**

---

```
'Put this in a module
Public dlocation As NADataStore
Public numpts As Long
Public fmt As NADataFormat
Public app As Application
Public measData As IArrayTransfer
Public chan As Channel

Sub Form_Load()
'Change analyzerName to your analyzer's full computer name
Set app = CreateObject("AgilentPNA835x.Application", "analyzerName")

Set measData = app.ActiveMeasurement
Set chan = app.ActiveChannel

'To pick a location to get the data from remove the comment from one of these
dlocation = naRawData
'dlocation = naCorrectedData
'dlocation = naMeasResult
'dlocation = naRawMemory
'dlocation = naMemoryResult

'setup MSChart1 and MSChart2
'right click on the chart and select:
' - line chart
' - series in rows
End Sub

Sub GetComplex_Click()
ReDim Data(numpts) As NAComplex
Dim Real(201) AS Single
Dim Imag(201) AS Single
numpts = chan.NumberOfPoints

'You cannot change the format of Complex Data
Call trigger
'get data
measData.GetNAComplex dlocation, numpts, Data(0)
```

```

'plot data
Dim i As Integer

For i = 0 To numpts - 1
 Real(i) = Data(i).Re
 Imag(i) = Data(i).Im
Next i
MSChart1 = Real()
MSChart2.Visible = True
MSChart2 = Imag()
Call Sweep
End Sub

```

```

Sub GetPaired_Click()
ReDim Real(numpts) As Single
ReDim Imag(numpts) As Single
numpts = chan.NumberOfPoints

```

```

' To pick a format, remove the comment from one of these
fmt = naLogMagPhase
'fmt = naLinMagPhase
Call trigger
'Get data
measData.getPairedData dlocation, fmt, numpts, Real(0), Imag(0)
'Plot Scalar
MSChart1 = Real()
MSChart2.Visible = True
MSChart2 = Imag()
Call Sweep
End Sub

```

```

Sub GetScalar_Click()
ReDim Data(numpts) As Single

```

```

numpts = chan.NumberOfPoints
'To pick a format remove the comment from one of these
fmt = naDataFormat_LogMag
'fmt = naDataFormat_LinMag
'fmt = naDataFormat_Phase
'fmt = naDataFormat_Delay
'fmt = naDataFormat_Real
'fmt = naDataFormat_Imaginary
Call trigger
'Get data
measData.GetScalar dlocation, fmt, numpts, Data(0)
'Plot Data
MSChart1 = Data()
MSChart2.Visible = False
Call Sweep
End Sub

```

```

Sub trigger()

```

```

'The analyzer sends continuous trigger signals
app.TriggerSignal = naTriggerInternal

```

```
'The channel will only accept one, then go into hold
'Sync true will wait for the sweep to complete
```

```
sync=True
```

```
chan.Single sync
End Sub
```

```
Sub Sweep()
'The channel goes back to accepting all triggers
chan.Continuous
End Sub
```

## Perform a Source Power Cal using COM

---

This program can be run in either Visual Basic 6 or as a VBScript program. The PNA can run \*.vbs programs as [macros](#).

This program demonstrates:

- Performing a source power calibration of Port 2 for Channel 1.
- Reading the calibration data.

Learn more about [Power Calibrations](#)

See an example that [Uploads a Source Power Cal](#)

### [See Other COM Example Programs](#)

To run this program, you need:

- One of the following power meters connected to the PNA through GPIB: E4416A, E4417A, E4418A/B, E4419A/B, 437B, 438A, EPM-441A, EPM-442A

---

**Note:** If your power meter is other than these, you can [create your own Power Meter Driver](#) using our template.

---

- Your PC and PNA both connected to a LAN (for communicating with each other).

To make this program work in VBS, save the following code in a text editor file such as Notepad and save as \*.vbs.

To make this program work in Visual Basic 6:

1. Create a new project
2. Click **Project, Add New Module**, click **Open**.
3. Paste the following code into the code window.
4. Delete the first two lines (comment and Main)
5. Click **Project, Properties**. Under **Startup Object**, select **Sub Main**
6. Click **Project, References**, and select the Agilent PNA Series Type Library.

```
' Run the Main subroutine
Main
Public Sub Main()
Dim PNA, chan, pwrCal
Const naPowerMeter = 0, naPowerMeterAndReceiver = 1
Const naPowerSensor_A = 0
Const naCorrectionValues = 0
Const port = 2
Const offset = 0
Const bDisplay = True
acquire
' PNA COM objects
' enum NASourcePowerCalMethod
' enum NAPowerAcquisitionDevice
' enum NASourcePowerCalBuffer
' PNA port #2 as source port
' cal power offset value
' whether to display data during
```

```

Dim stimulus, calvalues, strResult

' Instantiate our PNA COM objects
Set PNA = CreateObject("AgilentPNA835x.Application")
Set chan = PNA.Channels(1)
Set pwrCal = PNA.SourcePowerCalibrator

' Set the number of sweep points to 21 on Channel 1.
chan.NumberOfPoints = 21

' Specify the GPIB address of the power meter
' that will be used in performing the calibration.
pwrCal.PowerMeterGPIBAddress = 13

' Turn use of the loss table OFF (this assumes there is
' virtually no loss in the RF path to the power sensor
' due to a splitter, coupler or adapter).
pwrCal.UsePowerLossSegments = False

' Turn frequency checking OFF (so one power sensor is used for the entire cal
' acquisition sweep regardless of frequency span).
pwrCal.UsePowerSensorFrequencyLimits = False

' Specify a nominal power accuracy tolerance (IterationsTolerance) in dB for the
' calibration, and the maximum number of iterations to adjust power at each point,
' attempting to achieve within tolerance of the desired power. If at any stimulus
' point the power fails to reach within the set tolerance of the desired power
' after the maximum number of iterations, the power at that point will be set to the
' value determined by the last iteration (the Source Power Cal dialog box will
' indicate the FAIL, but we can still apply the cal if desired when it's complete).
' Each iteration is based upon a SETTLED power reading (see comments preceding the
' next two properties below).
pwrCal.IterationsTolerance = 0.1
pwrCal.MaximumIterationsPerPoint = 3

' The worst-case window of power uncertainty (for a calibration which meets
' tolerance) is the sum of the iteration tolerance and the power meter settling
' tolerance (which is described below).
' At each stimulus point, the PNA takes power meter readings and determines when
' they have settled by comparing the magnitude difference between consecutive
' readings versus a nominal dB tolerance limit (ReadingsTolerance) on that magnitude
' difference. When consecutive readings are within tolerance of each other, or
' if they are not within tolerance but we've taken a maximum number of readings
' (ReadingsPerPoint), the PNA does a weighted average of the readings taken at that
' stimulus point and that is considered our settled power reading.
pwrCal.ReadingsTolerance = 0.1
pwrCal.ReadingsPerPoint = 5

' Setup of information pertaining to this specific cal acquisition. Includes the
' method (type of devices) that will be used to perform the cal -- choose either
' naPowerMeter or naPowerMeterAndReceiver. naPowerMeterAndReceiver uses the power
' meter for the first iteration of each point and the PNA's reference receiver for
' subsequent iterations, so is much faster than using power meter only
naPowerMeter).
' But the power meter accounts for compression when calibrating at the output of an
' active device, whereas the reference receiver cannot unless it is coupled to the
' cal reference plane (on a PNA which allows direct access to the receivers).

```

```

' 'offset' specifies if the cal power level is offset (positive value for a gain,
' negative value for a loss) from the PNA port power setting on the channel when
' no source power cal is active. This is to account for components between the PNA
' test port and cal reference plane. In this example, we will calibrate at the PNA
' test port, so there is no offset (it is zero).
' 'bDisplay' indicates whether to display the source power cal dialog during the
' source power cal acquisition (the dialog will chart the corrected power readings).
pwrCal.SetCalInfo2 naPowerMeter, chan.ChannelNumber, port, offset, bDisplay

' Perform synchronous source power cal acquisition sweep using the sensor attached
' to Channel A of the power meter. This assumes that the power sensor is already
' connected to Port 2 of the PNA.
pwrCal.AcquirePowerReadings naPowerSensor_A, True

' Conclude the calibration. This applies the cal data to PNA channel memory,
' and turns the correction ON for Port 2 on Channel 1, but does NOT save the
' calibration.
pwrCal.ApplyPowerCorrectionValues

' At this point, if you choose to save the instrument state as a ".CST" file,
' the calibration will be saved with the instrument state in that file.
' Read the stimulus values from Channel 1.
stimulus = chan.GetXAxisValues

' Read the source power correction data.
calvalues = chan.getSourcePowerCalDataEx(naCorrectionValues, port)

' Print the data using a message box (here, Chr returns the ASCII characters
' for Tab (9) and Linefeed (10)).
strResult = "Stimulus" & Chr(9) & Chr(9) & "Cal Value" & Chr(10)
For i = 0 To UBound(stimulus)
strResult = strResult & stimulus(i) & Chr(9) & calvalues(i) & Chr(10)
Next
MsgBox strResult
End Sub

```

## Upload a Source Power Cal using COM

---

This program can be run in either Visual Basic 6 or as a VBScript program. The PNA can run \*.vbs programs as macros.

This program demonstrates:

- Uploading a source power calibration of Port 2 for Channel 1.
- Reading the calibration data.

Learn more about [Power Calibrations](#)

### **See Other COM Example Programs**

To run this program you need:

- Your PC and PNA both connected to a LAN (for communicating with each other).

To make this program work in VBS, save the following code in a text editor file such as Notepad and save as \*.vbs.

To make this program work in Visual Basic 6:

1. Create a new project
2. Click **Project, Add New Module**, click **Open**.
3. Paste the following code into the code window.
4. Delete the first two lines (comment and Main)
5. Click **Project, Properties**. Under **Startup Object**, select **Sub Main**
6. Click **Project, References**, and select the Agilent PNA Series Type Library.

```
' Run the Main subroutine
Main
Public Sub Main()
Dim PNA, chan ' PNA COM objects
Const naCorrectionValues = 0 ' enum NASourcePowerCalBuffer
Const port = 2 ' PNA port #2 as source port
Dim stimulus, calvalues
Dim power, calpower, strResult
' Instantiate our PNA COM objects
Set PNA = CreateObject("AgilentPNA835x.Application")
Set chan = PNA.Channels(1)

' Set the number of sweep points to 2 on Channel 1.
chan.NumberOfPoints = 2

' Ensure there's currently no source power cal on for this channel and port.
chan.SourcePowerCorrection(port) = False
```



```

' Specify if the cal power level is offset (positive value for a gain, negative
' value for a loss) from the PNA port power setting on the channel when
' no source power cal is active. This is to account for components
' between the PNA test port and cal reference plane.
' In this example, let's set up our calibration
' at the output of an amplifier with 15 dB gain.
chan.SourcePowerCalPowerOffset(port) = 15

' Send our source power correction data to the PNA. For purpose of simplicity
' in this example, we'll set up for no correction (0) at our start stimulus and
' 0.5 dB at our stop stimulus (recall that our sweep currently has just 2 points).
calvalues = Array(0, 0.5)
chan.putSourcePowerCalDataEx naCorrectionValues, port, calvalues

' Set the number of sweep points to 21 on Channel 1.
chan.NumberOfPoints = 21

' Read the fixed power level for this port on Channel 1.
power = chan.TestPortPower(port)

' Turn the source power cal on.
chan.SourcePowerCorrection(port) = True

' Again read the fixed power level for this port on Channel 1
' (with our calibration turned on, this should now include the 15 dB offset
' we indicated our power amplifier provides).
calpower = chan.TestPortPower(port)

' Read the stimulus values from Channel 1.
stimulus = chan.GetXAxisValues

' Read back the source power correction data, now interpolated for 21 points
calvalues = chan.getSourcePowerCalDataEx(naCorrectionValues, port)

' Print the data using a message box (here, Chr returns the ASCII characters
' for Tab (9) and Linefeed (10)).
strResult = "PNA port power = " & power & Chr(10)
strResult = strResult & "Power at reference plane = " & calpower & Chr(10) & Chr(10)
strResult = strResult & "Stimulus" & Chr(9) & Chr(9) & "Cal Value" & Chr(10)
For i = 0 To UBound(stimulus)
strResult = strResult & stimulus(i) & Chr(9) & calvalues(i) & Chr(10)
Next
MsgBox strResult
End Sub

```

## Upload Segment Table

---

This example program does the following:

- creates a 2-dimensional array (7 x 10) 7 data elements that define each segment x 10 segments
- uploads the data to the PNA

This program does not make sweep type = segment or show the segment table.

The comments indicate the order in which the segment elements are specified: Index 0 - segment state, Index 4 is IFBW, and so forth.

### See Other COM Example Programs

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save on the PNA hard drive as \*.vbs. [Learn how to setup and run the macro.](#)

```
' Create the application instance, and preset the application
Set app = CreateObject("AgilentPNA835x.Application")
app.Preset

Dim chan
Set chan = app.ActiveChannel
chan.sweepType = 4

Dim segs
Set segs = chan.Segments

Dim win
Set win = app.NAWindows(1)
win.ShowTable 2

' Multipliers
kHz = 1000
MHz = kHz*1000
GHz = MHz*1000
' Create segments from 10MHz to 3GHz
StartFreq = 10 * MHz
StopFreq = 3 * GHz
'*
'* Create 10 segments between StartFreq and StopFreq
'*
' Create a 2-D array of segments.
' 1st dimension is size 7 (6 is max index)
' to hold all the data per segment.
' 2nd dimension is size 10 (9 is max index)
' to hold 10 total segments.
Dim segdata(6, 9)
' Width of frequency segment, used below
SegmentWidth = (StopFreq-StartFreq)/10
```

```

' Fill up all 10 segments (indicies 0 to 9) with data
For i = 0 To 9
' element 0=segment state (on or off)
segdata(0, i) = True

' element 1=Num Points in this segment
segdata(1, i) = 500

' element 2=Start Freq
segdata(2, i) = StartFreq + i * SegmentWidth

' element 3=Stop Freq
segdata(3, i) = segdata(2, i) + SegmentWidth

' element 4=IFBW
segdata(4, i) = 35000

' element 5=Dwell Time
segdata(5, i) = 0

' element 6=Power
segdata(6, i) = 0

Next

' Configure Independent segment settings
segs.IFBandwidthOption = 1
segs.SourcePowerOption = 1

' Push the segment data into the PNA's Active Channel
segs.SetAllSegments segdata

```

## Create and Cal an SMC Measurement

---

This Visual Basic example creates and calibrates a scalar mixer measurement.

To run this example **without modification** you need the following:

- A Mixer setup file saved on the PNA: C:\Program Files\Agilent\Network Analyzer\Documents\Mixer\MyMixer.mxr.
- If the mixer file uses an external LO source, it must also be attached and configured.
- An ECAL module that covers the frequency range of the measurement.
- A power meter must be attached to the PNA. If this example is run in the PNA, the power meter does not need to be attached using a GPIB/USB interface.

The SCPI commands in this example are sent over a COM interface using the SCPIStringParser object. You do NOT need a GPIB connection to run this example. However, some modification is necessary to make the program run on a traditional GPIB Interface. For example, during the power meter portion of this calibration, scpi.Execute will not process a command until the power meter routine has completed. Traditional GPIB would require a serial polling technique to ensure the routine has completed before proceeding.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as SMC.vbs. Learn how to setup and run the macro.

```
Dim app
Dim scpi
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpIStringParser
'---Create a Scalar Mixer Forward Measurement
'First, delete all measurements on the channel
scpi.Execute "CALC:PAR:DEL:ALL"
'Create a forward scalar mixer measurement and configure it in
'channel 1. The first parameter is a unique
'identifying string (specified by the user) to allow subsequent
'commands to be directed at this specific measurement.
scpi.Execute "CALC:CUST:DEF ""My SC21"", ""SMC_Forward.SMC_ForwardMeas""
'For reverse measurements, use the following:
'scpi.Execute "CALC:CUST:DEF ""My SC12"", ""SMC_Reverse.SMC_ReverseMeas""
'Setup the new measurement as the 2nd trace in the active window
scpi.Execute "DISP:WIND:TRAC2:FEED ""My SC21""
'Make the new trace the active measurement
scpi.Execute "CALC:PAR:SEL ""My SC21""
'The parameters of the mixer measurement can now be configured.
'This can be done by either using the individual SENS:MIX commands
'for each of the parameters or by loading a mixer setup file. This
'example loads a mixer setup file. The path name
'for the mixer file may be loaded from other mapped drives
scpi.Execute "SENS:MIXer:Load ""C:\Program Files\Agilent\Network
Analyzer\Documents\Mixer\MyMixer.mxr""
'-----Perform A Scalar Mixer Calibration-----
'Initialize an SMC guided calibration for session number 6
scpi.Execute "SENS:CORR:COLL:SESS6:INIT ""SMC""
'Select to use an ECal for the 2-port cal portion of the procedure
'To use a mechanical kit you will have to use the following command:
'scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOPort:OPTION ""MECH""
```

```

scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOPort:OPTion ""ECAL""
'If you select the mechanical method then you also have to
'specify the connector types and the cal kits for each of the ports.
'The comments below show an example of how that is done:
'scpi.Execute "SENS:CORR:COLL:SESS6:CONN:PORT1:SEL ""APC 3.5 male""
'scpi.Execute "SENS:CORR:COLL:SESS6:CONN:PORT2:SEL ""APC 3.5 female""
'scpi.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT1:SEL ""85052D""
'scpi.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT2:SEL ""85052D""
'Specify the ECal module and the ECal characterization for this
'session. FCA calibrations currently only support ECal module
'number 1. In this example the factory characterization is used
'by specifying 0 for the characterization number.
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:ECAL:CHAR 1,0"
'Specify the thru measurement method. This applies to both ECal
'and mechanical calibrations. For ECal 'DEFAULT' will use the ECal
'thru. Other choices may be used depending on the genders and types
'of the connectors on the test interface.
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOP:METH ""DEFAULT""
'Omit the isolation part of the 2-port cal
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOP:OMIT 1"
'Turn on auto orientation for the ECal
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOP:ECAL:ORI:STATE 1"
'Set the Source port for the power cal to 1. If the
'measurement is an SMC Forward the valid port settings are '1' and
''BOTH' and if the measurement is an SMC Reverse, the valid port settings
'are '2' and 'BOTH'.
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:PWRC:SRCP ""1""
'Tell the wizard to generate and report the number of steps in this
'cal session
Dim steps
Dim desc
'Determine the number of steps required to complete the calibration.
'First send the write command, then the query.
scpi.Execute "SENS:CORR:COLL:SESS6:STEP"
steps = scpi.Execute ("SENS:CORR:COLL:SESS6:STEP?")
For i = 1 To steps
'Display the prompt for each step
desc = scpi.Execute ("SENS:CORR:COLL:SESS6:DESC? " & CStr(i))
MsgBox (desc)
'Perform the measurement for each step
scpi.Execute "SENS:CORR:COLL:SESS6:ACQ " & CStr(i)
Next
Dim calset
'Finish the cal and save the calset
calset = scpi.Execute ("SENS:CORR:COLL:SESS6:SAVE?")
Msgbox ("SMC Cal Complete!")

```

## Create and Calibrate a VMC Measurement

---

This VB Script example creates and calibrates a Vector mixer measurement. To run this example **without modification** you need the following:

- A Mixer setup file saved on the PNA: C:\Program Files\Agilent\Network Analyzer\Documents\Mixer\MyMixer.mxr.
- If the mixer file uses an external LO source, it must also be attached and configured.
- An ECAL module that covers the frequency range of the measurement.

The SCPI commands in this example are sent over a COM interface using the SCPIStringParser object. You do NOT need a GPIB connection to run this example. However, some modification may be necessary to make the program run on a traditional GPIB Interface.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as VMC.vbs. Learn how to setup and run the macro.

```
Dim app
Dim scpi
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpiStringParser
'---Create a Vector Mixer Measurement
'First, delete all measurements on the channel
scpi.Execute "CALC:PAR:DEL:ALL"
'Create a forward scalar mixer measurement and configure
'it in channel 1.
'The first parameter is a unique identifying string
'(specified by the user) to allow subsequent
'commands to be directed at this specific measurement.
SCPI.Execute "CALC:CUST:DEF "My VC21", "FCA.VMCMeas""
'Setup the new measurement as the 2nd trace in the active window
SCPI.Execute "DISP:WIND:TRAC2:FEED "My VC21""
'Make the new trace the active measurement
SCPI.Execute "CALC:PAR:SEL "My VC21""
'The parameters of the mixer measurement can now be configured.
'This can be done by either using the SENS:MIX commands
'for each of the parameters or by loading a mixer setup file.
'This example loads a mixer setup file. The path name
'for the mixer file may be loaded from other mapped drives.
SCPI.Execute "SENS:MIXer:Load "C:\Program Files\Agilent\Network
Analyzer\Documents\Mixer\MyMixer.mxr""

'-----Perform A Vector Mixer Calibration-----
'Initialize an VMC guided calibration for session number 6
SCPI.Execute "SENS:CORR:COLL:SESS6:INIT "VMC""
'This sets the VMC operation to full system cal as opposed to
'performing a mixer characterization only.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:OPER "CAL""
'This example uses ECAL for the 2-port cal portion of the procedure
'To use a mechanical kit you will have to use the following command:
'SCPI.Execute "SENS:CORR:COLL:SESS6:SMC:TWOport:OPTion"MECH""
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOport:OPTion "ECAL""
'If you select the mechanical method then you also have to
```

```

'specify the connector types and the cal kits for each of the ports.
'The comments below show an example of how that is done:
'SCPI.Execute "SENS:CORR:COLL:SESS6:CONN:PORT1:SEL ""APC 3.5 male""
'SCPI.Execute "SENS:CORR:COLL:SESS6:CONN:PORT2:SEL ""APC 3.5 female""
'SCPI.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT1:SEL ""85052D""
'SCPI.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT2:SEL ""85052D""
'Choose the between ECal or Mechanical calibration for the
'Mixer Characterization portion of the VMC cal.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:MIX:CHAR:CAL:OPT ""ECAL""
'This command sets the port mapping for the ECal to be used
'during the Mixer Characterization portion of the VMC cal.
'It is a required command if in the previous command the option
'was set to 'ECAL'. The only valid port maps are either 'A1'
'or 'B1'.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:MIX:ECAL:PORT 1, ""A1""
'Specify the ECal module and the ECal characterization for the
'two port calibration portion of this session. FCA calibrations
'currently only support ECal module number 1. In this example
'the factory characterization is used by specifying 0 for the
'characterization number.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:ECAL:CHAR 1,0"
'Specify the ECal module and the ECal characterization for the
'Mixer Characterization portion of this session. FCA calibrations
'currently only support ECal module number 1. In this example
'the factory characterization is used by specifying 0 for the
'characterization number.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:MIX:ECAL:CHAR 1,0"
'Specify the thru measurement method. This applies to both ECal
'and mechanical calibrations. For ECal 'DEFAULT' will use the ECal
'thru. Other choices may be used depending on the genders and types
'of the connectors on the test interface.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:METH ""DEFAULT""
'Omit the isolation part of the 2-port cal
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:OMIT 1"
'Turn on auto orientation for the ECal
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:ECAL:ORI:STATE 1"

'Tell the wizard to generate and report the number of steps in this
'cal session
Dim steps
Dim desc
'Determine the number of steps required to complete the calibration.
'First send the write command, then the query.
SCPI.Execute "SENS:CORR:COLL:SESS6:STEP"
steps = SCPI.Execute ("SENS:CORR:COLL:SESS6:STEP?")
For i = 1 To steps
 'Display the prompt for each step
 desc = SCPI.Execute ("SENS:CORR:COLL:SESS6:DESC? " & CStr(i))
 MsgBox (desc)
 'Perform the measurement for each step
 SCPI.Execute "SENS:CORR:COLL:SESS6:ACQ " & CStr(i)
Next
Dim calset
'Finish the cal and save the calset
calset = SCPI.Execute ("SENS:CORR:COLL:SESS6:SAVE?")
Msgbox ("VMC Cal Complete!")

```





## Create an SMC Fixed Output Measurement

---

This Visual Basic example creates a calibrated SMC fixed output measurement using a controlled LO. Then a single sweep is taken and data is retrieved.

Fixed output measurements are only supported on SMC (not VMC) measurements. Fixed output measurements require that an external LO source be sweeping and synchronized with the PNA source. FCA can perform this synchronization using the external source configuration settings. The fastest, and recommended, method of controlling the LO source is [Hardware List \(BNC\) triggering mode](#). However, in this mode, FCA channels will not respond to manual triggers. Therefore, the following example uses the "Single" [IChannel::Single](#) mechanism to trigger a sweep.

Both VMC and SMC measurements require that mixer parameters be setup before making the measurement. The mixer parameters are not applied until calling [IMixer::Calculate](#).

You can also setup the mixer parameters using [IMixer::LoadFile](#). With this interface, the specified mixer file is loaded and immediately applied.

```
option explicit
dim app
set app = createobject("agilentpna835x.application")
app.preset

' Put the channel in hold (highly recommended)
app.ActiveChannel.Hold 1

' Select calibration. Apply stimulus settings to the channel
app.ActiveChannel.SelectCalSet "{C9080B34-EF1F-4ED5-B07D-250B45962B99}",1

' Delete the standard measurement
app.ActiveMeasurement.Delete

' Create an SC21 measurement
app.CreateCustomMeasurementEx 1, "SMC_Forward.SMC_ForwardMeas","SC21"

' Set the number of points to 11
app.ActiveChannel.NumberOfPoints = 11

' Setup the mixer parameters for a swept LO, fixed output measurement

dim mixer
set mixer = app.ActiveMeasurement
mixer.InputStartFrequency = 200e6
mixer.InputStopFrequency = 700e6
mixer.LORangeMode(1) = 0 ' 0 = Swept mode
mixer.OutputFixedFrequency = 3.4e9
mixer.InputPower = -17
mixer.LOPower(1) = 10

' Specify the LO name, for controlled LO. This name can be setup in the External
Source Config Dialog
mixer.LOName(1) = "8360"

' The CALC method calculates the LO frequency from the other parameters,
' It also applies ALL mixer parameters to the channel.
mixer.Calculate 3 ' Calculate the LO range
```

```

' Create an S11 in the same channel
app.CreateCustomMeasurementEx 1, "SMC_Forward.SMC_ForwardMeas","S11"
dim S11Meas
set S11Meas = app.ActiveMeasurement

' Create an IPwr in the same channel
app.CreateCustomMeasurementEx 1, "SMC_Forward.SMC_ForwardMeas","IPwr"

' Create an OPwr in the same channel
app.CreateCustomMeasurementEx 1, "SMC_Forward.SMC_ForwardMeas","OPwr"

' Perform a single sweep synchronously.
app.ActiveChannel.Single 1
function ToString(complexDataArray)
dim dataAsString
dim point
for point = 0 to UBound(data)
dataAsString = dataAsString & "(" & data(point,0) & "," & data(point,1) & ") "
next
ToString = dataAsString
end function

' Retrieve the SC21 data
dim data
'Get the calibrated real/imaginary values
data = mixer.GetData(1,3)
wscript.echo ToString(data)

' Retrieve the S11 data
'Get the calibrated real/imaginary values
data = S11Meas.GetData(1,3)
wscript.echo ToString(data)

```

## Create a Pulsed Measurement

---

The following example demonstrates how to create a pulsed measurement using the Pulsed Application DLL. It first gets valid configuration settings and then uses those settings to configure the PNA and external pulsed generators.

To run this program, you need:

- [Pulsed Application](#) (Option H08)
- [IF Access](#) (Option H11)
- External Pulse Generators
- External Pulse Modulator / Pulse Bias

Learn how to [install and register the pulsed .dll](#) on your PC

See the [ConfigureNarrowBand3](#) Method for sending and returning parameters to the .dll.

See the documentation for the following [COM IF Configuration](#) commands.

See the [SCPI IF Configuration](#) commands.

Learn about the [Pulsed Application](#).

```
'Interfaces
```

```
Dim OApp As AgilentPNA835x.Application
Dim OIF As AgilentPNA835x.IFConfiguration
```

```
'Pulsed parameters
```

```
Dim DPRF As Double
Dim DOffset As Double
Dim DSampleRate As Double
Dim LNumTaps As Long
Dim LBW As Long
Dim IPrecision as Integer
Dim BPG81110 As Boolean
Dim BFixedPRF As Boolean
```

```
'pulsed DLL interface
```

```
Dim OPulsed As New AgilentPNAPulsed.Application
DPRF=5123 'Hz
LBW=100 'Hz
BPG81110=True 'Using the Agilent 81110A Pulse Generator
BFixedPRF=True 'Do not change the PRF during filter alignment. Only adjust the
IFBW.
```

```
'Calculate precision of pulse generators so that the config function returns the
correct precision with the right filter. For example, DPRF=5000 Hz with a pulse
generator that will only take a total of four numeric values
```

```
' (5.123 kHz)
'->log10(DPRF)=3.709
'->int(3.709)=3
'->3-3=0
```

```
'The algorithm will use a 10^x value for decrementing the PRF for null computation.
This means that the first numeric digit from the right should be the one that is
decremented by the pulsed algorithm (i.e. 5.122 kHz) to compute the filter nulls.
This ensures that the pulse generators receive a PRF that is within their precision
with the associated nulling IFBW.
```

```
IPrecision = Int(Flog10(CSng(DPRF))) - 3
```

```
'Send desired pulsed parameters to the pulsed configuration DLL. The DLL will return
a new set of pulse parameters that provide the proper filter nulling.
```

```
OPulsed.ConfigNarrowBand3 DPRF, LNumTaps, LBW, DOffset, DSampleRate, IPrecision,
BFixedPRF,BPG81110
```

```
'Send configuration to PNA
```

```
'Connect to the PNA application
```

```
Set OApp = CreateObject("AgilentPNA835x.Application")
```

```
Set OIF = OApp.ActiveChannel.IFConfiguration
```

```
'Set PNA IFBW close to that returned by pulsed algorithm. This ensures that the
proper settling time is set on the PNA.
```

```
OApp.ActiveChannel.IFBandwidth = LBW
```

```
OIF.IFFilterSamplePeriodMode = naMANUAL
```

```
OIF.IFFilterSamplePeriod = DSampleRate
```

```
OIF.IFFilterSource = naIFFilterSourceManual
```

```
OIF.IFFilterSampleCount = LNumTaps
```

```
OIF.IFGateEnable = True
```

```
OApp.ActiveChannel.FrequencyOffsetState = naON
```

```
OApp.ActiveChannel.FrequencyOffsetFrequency = DOffset
```

```
'Set receivers to medium gain setting
```

```
OIF.IFGainMode("ALL") = naMANUAL
```

```
OIF.IFGainLevel("A") = 1
```

```
OIF.IFGainLevel("B") = 1
```

```
OIF.IFGainLevel("R1") = 1
```

```
OIF.IFGainLevel("R2") = 1
```

```
Public Function Flog10(SGNum As Single) As Single
```

```
Flog10 = Log(SGNum) / Log(10)
```

```
End Function
```

```
'Enter Code here to send configuration to external pulse generators
```

## ECAL Confidence Check

---

This Visual Basic program:

- Initializes the PNA objects.
- Performs a complete ECAL confidence check

Before using this code:

- The active channel must contain an S11 measurement with a 1-port or N-port calibration
- Prepare a form with two buttons named **cmdRun** and **cmdQuit**

---

```
Private oPNA As AgilentPNA835x.Application
Private oChan As Channel
Private oCal As Calibrator
Private oMeas As Measurement

Private Sub cmdRun_Click()
Dim iMeasIndex As Integer

Set oPNA = CreateObject("AgilentPNA835x.Application", "MachineName")
Set oChan = oPNA.ActiveChannel
Set oCal = oChan.Calibrator

iMeasIndex = 1

' Loop through measurements until an S11 on the active channel
' is found, or the end of the measurement collection is reached.
Do
 Set oMeas = oPNA.Measurements(iMeasIndex)
 If oMeas.Parameter = "S11" And _
 oMeas.channelNumber = oChan.channelNumber Then Exit Do
 iMeasIndex = iMeasIndex + 1
 If iMeasIndex > oPNA.Measurements.Count Then
 MsgBox "No S11 measurement found on the active channel." _
 & " Create an S11 measurement, then try again."
 Exit Sub
 End If
Loop

' Set up trace view so we are viewing only the data trace.
```

---

```

oMeas.View = naData
' Acquire the S11 confidence check data from ECal Module A
' into the memory buffer.
oCal.AcquireCalConfidenceCheckECALEx "S11", 1
' Turn on trace math so the trace shows data divided by memory.
' You can be confident the S11 calibration is reasonably good if
' the displayed trace varies no more than a few tenths of a dB
' from 0 dB across the entire span.
oMeas.TraceMath = naDataDivMemory
End Sub

Sub cmdQuit_Click()
' Turn off trace math
' in case someone clicks Quit without having clicked Run
If oMeas <> Nothing Then oMeas.TraceMath = naDataNormal
' Conclude the confidence check to set the ECal module
' back to it's idle state.
If oCal <> Nothing Then oCal.DoneCalConfidenceCheckECAL
' End the program
End
End Sub

```

## Limit Line Testing with COM

---

This Visual Basic program:

- Turns off existing Limit Lines
- Establishes Limit Lines with the following settings:
  - Frequency range - 4 GHz to 8 GHz
  - Maximum value - (10dB)
  - Minimum value - (-30dB)
- Turns on Lines, Testing, and Sound

If using Global Pass/Fail to report limit results, trigger the PNA after configuring and enabling Limit lines.

```
Public limts As LimitTest
Set limts = meas.LimitTest
'All Off
For i = 1 To 20
 limts(i).Type = naLimitSegmentType_OFF
Next i

'Set up Limit Lines
limts(1).Type = naLimitSegmentType_Maximum
limts(1).BeginResponse = 10
limts(1).EndResponse = 10
limts(1).BeginStimulus = 4000000000#
limts(1).EndStimulus = 8000000000#
limts(2).Type = naLimitSegmentType_Minimum
limts(2).BeginResponse = -30
limts(2).EndResponse = -30
limts(2).BeginStimulus = 4000000000#
limts(2).EndStimulus = 8000000000#

'Turn on Lines, Testing, and Sound
limts.LineDisplay = 1
limts.State = 1
limts.SoundOnFail = 1
```

---

## COM Events Example

---

This Visual Basic program shows how to monitor the end of sweep.

The program will set sweep time to various amounts and BEEPs when sweep is completed. This method allows other processes to continue while waiting for end-of-sweep. This program stops after 10 loops.

---

**Note:** To avoid **Permission Denied** problems, this should be run on the PNA and not a PC. To run it from a PC both units must be "trusted" and on the same domain/workgroup.

---

```
Option Explicit
Dim na As AgilentPNA835x.Application
Dim WithEvents naEvt As AgilentPNA835x.Application
Dim ch As AgilentPNA835x.Channel
Dim sweepComplete As Boolean

Private Sub Form_Load()

Dim N As Integer
Set na = CreateObject("AgilentPNA835x.application")
na.preset
Set ch = na.ActiveChannel
na.DisallowAllEvents ' Turn off all events
Set naEvt = na ' Enable event interrupts
Do
N = N + 1 ' Loop counter
ch.sweepTime = 1 + (Rnd * 9) ' Set random sweep-time from 1-10 sec
sweepComplete = False
ch.Single False ' Trigger sweep
naEvt.AllowEventCategory naEventCategory_CHANNEL, True ' Enable Channel event
Do
DoEvents ' Allows other processes to continue
Loop Until sweepComplete = True
naEvt.AllowEventCategory naEventCategory_CHANNEL, False ' Disable event until
ready for next one
Beep ' Do end-of-sweep processing here;

Loop Until N > 10
End

End Sub

Private Sub naEvt_OnChannelEvent(ByVal eventID As Variant, ByVal chNumber As
Variant)
' In this example we don't care about the channel info
If eventID = naEventID_CHANNEL_TRIGGER_COMPLETE Then sweepComplete = True
End Sub
```



## Configure for COM-DCOM Programming

---

Before developing or running a COM program, you should first establish communication between your PC and the analyzer. This process is referred to as gaining **Access** to the analyzer. You should then register the PNA type library on your PC.

**DCOM** (Distributed Component Object Model) refers to accessing the PNA from a remote PC.

**COM** refers to accessing the PNA application from the analyzer PC.

### [Access Concepts](#)

### [Access Procedures](#)

### [Register the PNA Type Library on Your PC](#)

### [Problems?](#)

---

**Note:** After performing a [Firmware Upgrade](#) you must copy the new type library to your development PC to get access to new COM commands. See [Register the analyzer on your PC](#).

---


## Other Topics about COM Concepts

For detailed information on this subject, see <http://na.tm.agilent.com/pna/DCOMSecurity.html>

## Access Concepts

PNAs are shipped from the factory such that **Everyone** has permission to launch and access the PNA application via COM/DCOM. The term **Everyone** refers to a different range of users depending on whether the PNA is a member of a **Domain** or **Workgroup** (it must be one or the other; not both). By default, the PNA is configured as members of a workgroup. Therefore, **Everyone** includes only those users who have been given logon accounts on the PNA.

### Workgroup

 A workgroup is established by the **PNA administrator** declaring the workgroup name and declaring the PNA as a member of the workgroup. A workgroup does not require a network administrator to create it or control membership.

**Everyone** includes only those users who have been given logon accounts on the PNA.

By default, the PNA is configured as members of a workgroup named WORKGROUP.

---

**Note:** To setup a logon account for a new user, see [Additional Users](#).

The easiest method of gaining DCOM access, is to make the user's account name and password on the PNA to EXACTLY match their PC logon account name and password.

---

### Domain

A domain is typically a large organizational group of computers. Network administrators maintain the domain and control which machines have membership in it.

**Everyone** includes those people who have membership in the domain. In addition, those with logon accounts can also access the analyzer.

### Summary

- A **Workgroup** requires no maintenance, but allows DCOM access to only those users with a log-on account for the PNA.
- A **Domain** requires an administrator, but all members of the domain and those with logons to the analyzer are allowed DCOM access to the PNA.

The following section "Access Procedures" provides a tighter level of security allowing only **selected** (not **Everyone**) domain and workgroup users DCOM **Access** and **Launch** capability of the PNA.

## Access Procedures

Perform this procedure for the following reasons:

- To allow only selected users (not everyone) remote Access and remote Launch capability to the PNA. Launch capability is starting the PNA application if it is not already open.
- To verify that you have DCOM access to the analyzer.

---

**Note:** Before doing this procedure, you must first have a logon account on the PNA. See [PNA User Accounts](#)

---

**The following procedure grants specific users DCOM access and launch capability of the PNA application:**

To perform this procedure, you must first [minimize the PNA](#) application.

How do I know which Operating System I have?

| Windows 2000                                                                                                                                         | Windows XP                                                                                                                                                                                            |
|------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| On the PNA, click the Windows <b>Start</b> button                                                                                                    | On the PNA, click the Windows <b>Start</b> button                                                                                                                                                     |
| Click <b>Run</b>                                                                                                                                     | Click <b>Run</b>                                                                                                                                                                                      |
| In the <b>Open:</b> box, type <b>dcomcnfg</b>                                                                                                        | In the <b>Open:</b> box, type <b>dcomcnfg</b>                                                                                                                                                         |
| Click <b>OK</b>                                                                                                                                      | Click <b>OK</b>                                                                                                                                                                                       |
| In the Distributed COM Configuration Properties window, Click on <b>Agilent PNA Series</b> in the Applications list. Then click <b>Properties...</b> | Open the following folder sequence:<br>Component Services Window<br>Component Services<br>Computers<br>My Computer<br>DCOM Config<br>Right click <b>Agilent PNA Series</b><br>Click <b>Properties</b> |
| Click the <b>Security</b> tab                                                                                                                        | Click the <b>Security</b> tab                                                                                                                                                                         |
| Click <b>Use custom access permissions</b> then click <b>Edit</b>                                                                                    | Under <b>Access Permissions</b> , click <b>Customize</b> , then click <b>Edit</b>                                                                                                                     |

|                                                                                                                                                                                                                                                                                                                                                                    |                                                                                   |
|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------|
| In <b>Registry Value Permissions</b> , select <b>Everyone</b> , then click <b>Remove</b>                                                                                                                                                                                                                                                                           | Select <b>Everyone</b> , then click <b>Remove</b>                                 |
| Click <b>Add</b>                                                                                                                                                                                                                                                                                                                                                   | Click <b>Add</b>                                                                  |
| You could either select one or more of these groups to have access to the PNA, or specific users. To give specific users access, click <b>Show users</b> or <b>Members</b> , then select the name from the list.                                                                                                                                                   | Type a group name or user account name                                            |
| Click <b>Add</b> , then click <b>OK</b>                                                                                                                                                                                                                                                                                                                            | Click <b>OK</b>                                                                   |
| <b>Launch Permission</b>                                                                                                                                                                                                                                                                                                                                           |                                                                                   |
| Click <b>Use custom launch permissions</b> , then click <b>Edit</b>                                                                                                                                                                                                                                                                                                | Under <b>Launch Permissions</b> , click <b>Customize</b> , then click <b>Edit</b> |
| In Registry Value Permissions, select <b>Everyone</b> then click <b>Remove</b>                                                                                                                                                                                                                                                                                     | Select <b>Everyone</b> , then click <b>Remove</b>                                 |
| Click <b>Add</b>                                                                                                                                                                                                                                                                                                                                                   | Click <b>Add</b>                                                                  |
| You could either select one or more of these groups to have launch permission of the PNA, or specific users. <ul style="list-style-type: none"> <li>To give groups launch permission, select the group from the list.</li> <li>To give specific users launch permission, click <b>Show users</b> or <b>Members</b>, then select the name from the list.</li> </ul> | Type a group name or user account name                                            |
| Click <b>Add</b> , then click <b>OK</b>                                                                                                                                                                                                                                                                                                                            | Click <b>OK</b>                                                                   |

## Register the PNA Type Library on Your PC

The type library contains the PNA object model. On your PC, there is a Registry file that keeps track of where object models are located. Therefore, you must register the type library on the PC that will be used to develop code and run the program. It is much more efficient to have the type library registered at design time (BEFORE running your COM program).

Do the following two items before proceeding:

1. Connect your PC and the PNA to LAN.
2. Either map a drive to the analyzer or copy the type library files on a floppy disk or other media. See [Drive Mapping](#).

---

**Note:** To register the type library on your PC, you must be logged on as an administrator of your PC. Learn about [User Accounts](#).

---

This procedure will do the following:

- Register the Network Analyzer application on your PC.

- Copy and register the proxystub (835xps.DLL) onto the PC.
  - Copy and register the PNA type library (835x.tlb) onto the PC.
  - Copy and register the FCA type library (fca.tlb) onto the PC.
1. Using Windows Explorer on your PC, find the Analyzer's C: drive. The drive will not be named "C:" on your PC, but a letter you assigned when mapping the drive.
  2. Navigate to **Program Files \ Agilent \ Network Analyzer \ Automation**
  3. Double-click **pnaproxy.exe** and follow the prompts to Install PNA Proxy. If the installation offers a choice of Modify, Repair, or Remove, then select **Remove**. Then double-click on **pnaproxy.exe** again.
  4. When prompted, type the Computer name of the PNA ([Learn how to find this](#)).
  5. After the install program runs, the PNA and FCA type library should be registered on your PC.
  6. Your programming environment may require you to set a reference to the PNA type library now located on your PC. In Visual Basic, click **Project, References**. Then browse to **C:\Program Files\Common Files\Agilent\PNA**  
Select **835x.tlb**

#### Problems?

- These procedures will fail if there are any programs using the PNA type library (for example: Visual basic, VEE, Visual Studio, or any other application program that may communicate with the PNA).
  - Perform the following procedure if the previous procedure did not return an error, but you cannot connect to the PNA.
  - If you received an error, check that both the account name and password used on both the PNA and PC match EXACTLY.
  - If you still get errors, see <http://na.tm.agilent.com/pna/DCOMSecurity.html>.
1. Map a drive from your remote PC to the PNA. Note the drive letter your PC assigns to the PNA. Substitute this drive letter for **PNA** in the following procedure.
  2. On your PC, go to a DOS prompt c:>
  3. Type **PNA:** (for example o:)
  4. Type **cd program files\agilent\network analyzer\automation**
  5. Type **copy 835xps.dll c:\program files\common files\agilent\pna**
  6. Type **copy 835x.tlb c:\program files\common files\agilent\pna**

If you will NOT be using FCA commands, skip steps 6, 7,.8.

6. Type **cd..**
7. Type **cd applications\fca**
8. Type **copy fca.tlb c:\program files\common files\agilent\pna**

9. If it is not already there, copy **regtlib.exe** from **PNA:\WINNT** to your C:\<windows>\system32 directory (<windows> is OS-dependent- it is either windows or WINNT)
0. Type **regtlib C:\program files\common files\agilent\pna\835x.tlb**
1. Type **regsvr32 C:\program files\common files\agilent\pna\835xps.dll**
2. Type **regtlib C:\program files\common files\agilent\pna\fca.tlb**

Perform the Access Procedure after doing these steps.

## COM Fundamentals

---

The following terms are discussed in this topic:

[Objects](#)

[Interfaces](#)

[Collections](#)

[Methods](#)

[Properties](#)

[Events](#)

[Visual Basic Syntax](#)

---

**Note:** The information contained in this topic is intended to help an experienced SCPI programmer transition to COM programming. This is NOT a comprehensive tutorial on COM programming.

---

### Other Topics about COM Concepts

#### Objects

The objects of the Network Analyzer (Application) are arranged in a hierarchical order. The [Network Analyzer object model](#) lists the objects and their relationship to one another.

In SCPI programming, you must first select a measurement before making settings. With COM, you first get a handle to the object (or collection) and refer to that object in order to change or read settings (properties).

For more information on working with objects, see [Getting a Handle to an Object](#).

#### Interfaces

A COM Interface is the connection to an object. When you get a handle to an object, you are actually using an interface to an object. This is important if you are developing PNA code that will run on multiple code versions. For more information, see [PNA Interfaces](#).

#### Collections

A collection is an object that contains several other objects of the same type. For example, the **Channels** collection contains all of the channel objects.

---

**Note:** In the following examples, the collections are referred to as a variable. Before using a collection object, you must first get an instance of that object. For more information, see [Getting a Handle to an Object](#)

---

Generally, items in a collection can be identified by **number** or by **name**. The order for objects in a collection cannot be assumed. They are always unordered and begin with 1. For example, in the following procedure, chans(1) is used to set averaging on the **first** channel in the Channels collection (not necessarily channel 1).

```
Sub SetAveraging()
 chans(1).AveragingFactor = 10
End Sub
```

The following procedure uses the measurement string name to set the display format for a measurement in the measurements collection.

```
meass("CH1_S11_1").Format = 1
```

---

You can also manipulate an entire collection of objects if the objects share common methods. For example, the following procedure sets the dwell time on all of the segments in the collection.

```
Sub setDwell()
For Each seg In segs
 segs.DwellTime = 0.03
Next
End Sub
```

## Methods

A method is an action that is performed on an object. For example, **CreateSParameter** is a method on the [Application](#) object. The following procedure uses that method to create a new S21 measurement in channel 1 in a new window.

```
Sub CreatMeas
 app.CreateSParameter 1,2,1,1
End Sub
```

## Properties

A property is an attribute of an object that defines one of the object's characteristics, such as size, color, or screen location. A property can also change an aspect of the object's behavior, such as whether the object is visible. In either case, to change the characteristics of an object, you change the values of its properties.

For example, the following statement sets the IF Bandwidth of a channel to 1 KHz.

```
Chan.IFBandwidth = 1e3
```

You can also read the current value of a property. The following statement reads the current IF Bandwidth of a channel into the variable **ifbw**.

```
Ifbw = Chan.IFBandwidth
```

Some properties cannot be set and some cannot be read. The Help topic for each property indicates if you can:

- Set and read the property (Write/Read)
- Only read the property (Read-only)
- Only set the property (Write-only)

## Events

An event is an action recognized by an object, such as clicking the mouse or pressing a key. Using events, your program can respond to a user action, program code, or triggered by the analyzer. For example:

```
OnChannelEvent
```

For more information, see [Working with the Analyzer's Events](#).

## Visual Basic Syntax

The examples in PNA Help use Visual Basic as the programming environment, which uses 'dot' notation.

To set a property, an object, or reference to an object is followed with:

- a period (.)
- property or method
- an equal sign (=)
- the new value

For example:

```
object.property = value 'This Green text following an apostrophe (') is a comment.
```

To read a property, a variable to contain the returned value is followed with:

- an equal sign (=)
- an object, or reference to an object
- a period (.)
- property

For example:

```
variable = object.property
```

To execute a method, an object, or reference to an object is followed with:

- a period (.)
- the method
- a blank space
- any required parameters

For example:

```
object.method parameters
```

Some methods return values, such as methods that return data. To return data from a method, a variable to contain the returned data is followed with:

- an equal sign (=)
- an object, or reference to an object
- a period (.)
- the method
- any required parameters enclosed in parenthesis

```
variable = object.method (parameters)
```



## Getting a Handle to an Object

---

The following are discussed in this topic:

### [What Is a Handle](#)

### [Declaring an Object Variable](#)

### [Assigning an Object Variable](#)

### [Navigating the Object Hierarchy](#)

### [Getting a Handle to a Collection](#)

## Other Topics about COM Concepts

### What Is a Handle

In SCPI programming, you must first select a measurement before changing or reading settings. With COM, you first get a handle to the object (or collection) and refer to that object to change or read its settings. The following analogy illustrates this:

A CAR could be called an object. More precisely, CAR is a class of objects. For example, one of the properties of the CAR class is "**Color**". You can read (by looking) or set (by painting) the color property of A car object. In other words, you can only read or set properties of a specific car object; not the entire car class. Therefore, to read or set a property, you need to get "a handle", or an instance of the object.

This process is also called "accessing an object", "getting an instance of an object", "returning an object". or "referring to an object". You can have handles to many instances of an object at the same time.

### Accessing PNA Objects

The PNA Application object is the highest object in the PNA object model hierarchy. Because of that, it is the only object that must be 'created' before it, or any other objects, can be accessed and used. During the creation process, the application object assigned to a variable name, or handle. Throughout your program, that object is used by referring to that variable. All PNA objects can be assigned to a variable, and subsequently referred to, in this same manner.

The following example shows how to create the PNA Application object, as well as illustrate the general steps of get a handle to an object.

There are two steps in the process of getting a handle to analyzer objects:

1. Declaring a Variable
2. Assigning an Object to the Variable

#### 1. Declaring a Variable

**Note:** The examples in these topics use the Visual Basic Programming Language. See the short section regarding [Visual Basic syntax](#).

Use the Dim statement or one of the other declaration statements (Public, Private, or Static) to declare a variable. The type of variable that refers to an object must be a Variant, an Object, or a specific type of object. Some programming languages, such as VBScript and Agilent VEE, do not allow you to specify variable types.

The following examples ALL declare the variable **pna**. Each subsequent statement is more specific than the previous:

- `Dim pna 'Variant data type.`
- `Dim pna As Object 'Object data type.`
- `Dim pna As AgilentPNA835x.Application ' Specific Application type`
- `Dim pna As AgilentPNA835x.IApplication ' Interface type`

1. If you use a variable without declaring it first, the data type of the variable is Variant. If you don't care about using automatic type checking, and willing to run code less efficiently, this method is very safe and is useable on all programming environments.
2. If you know the specific object type, and your programming environment allows it, you can declare the variable as an object.
3. Declaring a specific object type provides automatic type checking (Intellisense), faster code, and improved readability.
4. Declaring the interface is the most specific way and is beneficial when developing code for multiple firmware revisions. [Learn more about Interfaces.](#)

## 2. Assigning an Object to a Variable

To assign an object instance to a variable, use the **Set** keyword before the object variable that was declared previously. In the following line of code, we SET the current AgilentPNA835x Application to "pna".

```
Set pna = AgilentPNA835x.Application
```

As mentioned earlier, the AgilentPNA835x object is unique because it is the highest level of object in the PNA object model hierarchy. Therefore, we must use the **CreateObject** keyword with the (*classname,server name*) parameters.

- The **classname** for the analyzer object is always "AgilentPNA835x.Application".
- To find your analyzer's **server name**, see [View or change full computer name](#)

The following statements create an instance of the Analyzer object.

```
Dim pna AS AgilentPNA835x.Application
Set pna = CreateObject("AgilentPNA835x.Application", "Analyzer46")
```

---

**Note:** These statements will start the PNA application if it is not already running on your instrument.

---

## Navigating the Object Hierarchy

Once an instance of the PNA Application is "created", you access all of the PNA objects by navigating the object hierarchy. Navigating the object model hierarchy can be tricky. In addition, you also need to know how to refer to a specific instance of that object. For example, if you have three measurements present on the PNA, how do you refer to the channel 1 measurement? Each object on the PNA Object Model image is linked to an object page. At the top of each object page is a **Description** section and another called "**Accessing the ... Object**". These sections together explain how to navigate the PNA hierarchy to access a specific instance of that object.

From the previous discussion, you may think that you must always declare and assign variables to an object before setting or reading its properties. While this method is best for objects that you will continue to reuse, such as a measurement, it is not always necessary. You can also refer to an object directly.

The [TriggerSetup](#) object, which is a child of the Application object. Because we will only need to refer to this object once to set a couple of properties, and it is easy to access, we will refer to it directly. From the previous example, we already have a handle to the Application object in the variable **pna**. The following example uses [Visual basic 'dot' notation](#) to refer to the TriggerSetup object, and then the Scope property.

```
pna.TriggerSetup.Scope = naChannelTrigger
```

By referring to the TriggerSetup object directly, we must type the same path whenever we refer to properties on the TriggerSetup object. The following method assigns the pna.TriggerSetup object to a variable that can be reused.

```
Dim trig As Object
Set trig = pna.TriggerSetup
```

Once created, you can treat an object variable exactly the same as the object to which it refers. For example:

```
trig.Scope = naChannelTrigger
trig.Source = naTriggerSourceInternal
```

### Getting a Handle to a Collection

The analyzer has several collections of objects which provide a convenient way of setting or reading all of the objects in the collection with a single procedure. Also, there are objects (limit lines for example) that can only be accessed through the collection.

To get a handle to an item in a collection, you can refer to the object by item number or sometimes by name. However, you first have to get a handle to the collection. To assign the collection to a variable, use the same two step process (1. declare the variable, 2. assign the variable using 'Set').

```
Dim meass As Measurements
```

```
Dim meas As Measurement
```

You can then iterate through the entire collection of measurements to read or set properties

```
Sub setFormat()
For Each meas In meass
 meas.Format = naDataFormat_LinMag
Next
End Sub
```

Or you can read or set a property on an individual object in the collection:

```
meass(1).Format = naLinMag
```

**Note:** Each object and collection has its own unique way of dealing with item names, and numbers. Refer to the [Analyzer Object Model](#) for details.

---

## Collections in the Analyzer

---

Collections are a gathering of similar objects. They are a convenience item used primarily to iterate through the like objects in order to change their settings. Collections generally provide the following generic methods and properties:

```
Item(n)
Count
Add(n)
Remove(n)
```

where **(n)** represents the number of the item in the collection. Some collections may have unique capabilities pertinent to the objects they collect.

### Other Topics about COM Concepts

---

#### Collections are Dynamic

**A collection does not exist until you ask for it.** When you request a Channels object (see Getting a Handle to an Object / [Collection](#)), handles to each of the channel objects are gathered and placed in an array.

For example, if channels 2 and 4 are the only channels that exist, then the array will contain only 2 items. The command 'channels.Count' will return the number 2, and:


- Channels(1) will contain the channel 2 object.
- Channels(2) will contain the channel 4 object.

**The ordering of objects within the collection should not be assumed.** If you add a channel to the previous example, as in:

```
Pna.Channels.Add(3)
```

'channels.Count' will now return 3 and:

- Channels(1) will contain the channel 2 object.
- Channels(2) will contain the channel 3 object.
- Channels(3) will contain the channel 4 object.

 Primarily, collections are useful for making this type of iteration possible:

```
Dim ch as Channel
For each ch in pna.Channels
 Print ch.Number
 Print ch.StartFrequency
 Print ch.StopFrequency
Next ch
```

As soon as this for-each block has been executed, the Channels object goes out of scope.

---

## COM Data Types

---

The PNA uses several data types to communicate with the host computer. Before using a variable, it is best to declare the variable as the type of data it will store. It saves memory and is usually faster to access. The following are the most common data types:

[Long Integer](#)

[Single Precision \(Real\)](#)

[Double Precision \(Real\)](#)

[Boolean](#)

[String](#)

[Object](#)

[Enumeration](#)

[Variant](#)

---

### Other Topics about COM Concepts

---

**Long** (long integer) variables are stored as signed 32-bit (4-byte) numbers ranging in value from -2,147,483,648 to 2,147,483,647.

---

**Double** (double-precision floating-point) variables are stored as IEEE 64-bit (8-byte) floating-point numbers ranging in value from -1.79769313486232E308 to -4.94065645841247E-324 for negative values and from 4.94065645841247E-324 to 1.79769313486232E308 for positive values.

---

**Single** (single-precision floating-point) variables are stored as IEEE 32-bit (4-byte) floating-point numbers, ranging in value from -3.402823E38 to -1.401298E-45 for negative values and from 1.401298E-45 to 3.402823E38 for positive values.

---



**Boolean** variables are stored as 16-bit (2-byte) numbers, but they can only be True or False. Use the keywords True and False to assign one of the two states to Boolean variables.

When other numeric types are converted to Boolean values, 0 becomes False and all other values become True. When Boolean values are converted to other data types, False becomes 0 and True becomes -1.

---

**String** variables hold character information. A String variable can contain approximately 65,535 bytes (64K), is either fixed-length or variable-length, and contains one character per byte. Fixed-length strings are declared to be a specific length. Variable-length strings can be any length up to 64K, less a small amount of storage overhead.

---

**Object** variables are stored as 32-bit (4-byte) addresses that refer to objects within the analyzer or within some other application. A variable declared as Object is one that can subsequently be assigned (using the Set statement) to refer to any actual analyzer object.

---

**Enumerations (Enum)** are a set of named constant values. They allow the programmer to refer to a constant value by name instead of by number. For example:

---

```
Enum DaysOfWeek
 Sunday = 0
 Monday = 1
 Tuesday = 2
 Wednesday = 3
 Thursday = 4
 Friday = 5
 Saturday = 6
End Enum
```

Given this set of enumerations, the programmer can then pass a constant value as follows:

```
SetTheDay(Monday)
```

rather than

```
SetTheDay(1)
```

where the reader of the code has no idea what the value 1 refers to.

However, the analyzer RETURNS a long integer, not the text.

```
Day = DaysOfWeek(today) 'Day = 1
```

---

**Variant** - If you don't declare a data type ("typed" data) the variable is given the Variant data type. The Variant data type is like a chameleon — it can represent many different data types in different situations.

The PNA provides and receives Variant data because there are programming languages that cannot send or receive "typed" data. Variant data transfers at a slower rate than "typed" data.

---

## PNA Interfaces

---

A COM interface is the connection to an object. When you get a handle to an object, you are actually using an interface to an object. This subtle distinction is relevant to the COM programmer for the following two reasons:

### Interface Inheritance (Coding for Multiple PNA Versions)

#### Custom Interfaces.

### Other Topics about COM Concepts

### Interface Inheritance (Coding for Multiple PNA Versions)

The PNA continues to evolve and release new firmware / software versions that provide more functionality and features. New commands are added to existing objects, and with them new interfaces are added to support those commands. For example, new commands were added to the Measurement object in PNA release 3.0. These commands are accessible from the new IMeasurement2 interface. This can be important if you develop code using the type library in release 3.0, and run the code on a PNA with an older release, such as 2.0

When you use a command that was new with release 3.0, and you run that code on a PNA with release 2.0 firmware, errors will occur because that PNA does not recognize the new commands. However, even if you do NOT utilize new commands, errors can still occur. The following example shows how this occurs and how to avoid it.

The following Visual Basic statement dimensions the **meas** variable as an object.

```
Dim meas As Measurement
```

When the program compiles, Visual Basic figures out what interface to use to access that object. When dimensioning as an object, VB will use the default interface. As new interfaces are added to an object, they become the default interface. If this program was developed and compiled using the PNA 3.0 type library, the default Interface of the Measurement Object was IMeasurement2. However, if this program is run on an instrument with PNA 2.0 firmware, there was no IMeasurement2 Interface, and an E\_NOINTERFACE error will occur.

Therefore, the more robust approach would be to specify the interface instead of the object when declaring a variable.

```
Dim meas As IMeasurement
```

This code will ONLY use the IMeasurement interface; not the default interface.

However, regardless of how you declare a variable, errors will always occur if you use new commands, and run the code on an older instrument.

### Custom Interfaces

The PNA object model contains three "custom" interfaces. These interfaces allow the Visual Basic and C++ programmer to transfer data using "typed" variables, which is more efficient than using variant type variables. These interfaces are:

- IArrayTransfer - Measurement object
- ICalData - Calibrator object
- ISourcePowerCalData - Channel object

## Working with Events

---

### [What are Events?](#)

### [Using the Analyzer's Events](#)

### [Event ID's](#)

### [Filtering Events](#)

### [List of Events](#)

### [Out of Range Errors](#)

### [Troubleshooting Problems with Events](#)

See [Events Example](#).

## Other Topics about COM Concepts

### What are Events?

Windows applications work from user-initiated events such as mouse moves and mouse clicks. A mouse-click produces an event that the programmer can either ignore or "handle" by providing an appropriate subroutine like this:

```
Sub DoThis_onClick
 Perform something
End Sub
```

If this subroutine were in your program and the mouse-click event occurs on your PC, it would generate a "Callback" to the client and interrupt whatever it was doing and handle the event.

A more practical example of an event in the analyzer is Limit test. If limit test is on and the measurement fails, the analyzer produces a "Limit-failed" event. If the measurement passed, the analyzer produces a "Limit-succeeded" event.

The Analyzer has a very sophisticated Event structure. Your program **CAN** be notified when one or more events occur. However, it may not be necessary.

For example, the analyzer has an event that will notify your program when a sweep is complete. A simpler alternative is to use a synchronous command which waits for the sweep to complete.

```
sync = True
app.ManualTrigger sync
chan.StartFrequency = 4.5E6
```

This would NOT work if you want the controller to do other things while waiting, like setup a power meter or sort some data. In this case you would like a "callback" from the analyzer to let your program know that the sweep has completed. For an example of this see [Events Example](#).

Another reason to use events is when you want to be notified of several conditions when they occur, such as errors or source unlock conditions. It would not be practical to routinely poll these conditions while executing your program.

---

### Using Events

If you decide to use the COM events to get a callback, your program must do two things:





| Code | Severity Enumeration                                                                         |
|------|----------------------------------------------------------------------------------------------|
| 00   | naEventSeveritySUCCESS - the operation completed successfully                                |
| 01   | naEventSeverityINFORMATIONAL - events that occur without impact on the measurement integrity |
| 10   | naEventSeverityWARNING - events that occur with potential impact on measurement integrity    |
| 11   | naEventSeverityERROR - events that occur with serious impact on measurement integrity        |

### List of Events

The following is a list of categories and the general types of events they include. Click the link view the event details.

| Category Enumeration    | Callback                           |
|-------------------------|------------------------------------|
| naEventCategory_PARSER  | <a href="#">OnSCPIEvent</a>        |
| naEventCategory_MEASURE | <a href="#">OnMeasurementEvent</a> |
| naEventCategory_CHANNEL | <a href="#">OnChannelEvent</a>     |
| naEventCategory_HW      | <a href="#">OnHardwareEvent</a>    |
| naEventCategory_CAL     | <a href="#">OnCalEvent</a>         |
| naEventCategory_USER    | <a href="#">OnUserEvent</a>        |
| naEventCategory_DISPLAY | <a href="#">OnDisplayEvent</a>     |
| naEventCategory_GENERAL | <a href="#">OnSystemEvent</a>      |

**Note:** Use the [MessageText](#) Method to get a text message describing the event.

### Out of Range Errors

When you attempt to set a value on an active function that is beyond the range (min or max) of the allowable values, the analyzer limits that value to an appropriate value (min or max) and sets the function to the limited value. From the front panel controls this is visually evident by the limited value in the edit box or by the annotation on the display. An example would be attempting to set the start frequency below 300kHz. The edit control doesn't allow the number to fall below 300kHz.

When the automation user programs a setting (such as start frequency below the allowable limits) the same behavior takes place. The analyzer accepts the limited value. However, in order to learn what setting took place, you have to read the HRESULT.

All automation calls return HRESULTS. By default the HRESULT returned when an overlimit occurs is S\_NA\_LIMIT\_OUTOFRANGE. This value is a success code, meaning that bit 31 in this 32 value is 0. Programmers should check the return code from all automation calls to determine success or failure.

Some C++ macros (like SUCCEEDED(hr) or FAILED(hr) ) only check bit 31. So if you are interested in trapping this outOfRange error you will have to check for S\_NA\_LIMIT\_OUTOFRANGE explicitly.

Alternatively, you can configure the analyzer to report outOfRange conditions with an error code. Use the method: [App.SetFailOnOverRange](#) (true). With this method set TRUE, any overrange error will return E\_NA\_LIMIT\_OUTOFRANGE\_ERROR.

This method is provided for the benefit of VB clients. VB users can't detect specific success codes because the VB runtime strips off the HRESULT and only raises a run time error if bit 31 is set, indicating a fail code.

---

## Troubleshooting Problems with Callbacks

When you do callbacks, the client PC becomes the server and the analyzer (server) becomes the client. Callbacks can only take place when both server and client are in the same workgroup or in the same domain. See [Configure for COM](#).

## Read and Write Calibration Data using COM

---

Calibration data in the PNA is stored in Cal Sets. [Learn more about Cal Sets](#)

You can read or write two types of Calibration data:

- **Error Terms** - calculated data using standard measurement data and the algorithms for the specified cal type.
- **Standard Measurement data** -raw data resulting from the measurement of a calibration standard.

Each of these data are available in the PNA in either variant data or typed data. [Learn more about variant and typed data](#)

### Other Topics about COM Concepts

#### Calibration / Cal Set Interfaces

There are several interfaces associated with Calibration.

##### ICalibrator

This interface is the original interface provided with the first version of the PNA. It provides remote access to the "Unguided" Calibration wizard. This interface can perform 1 and 2 port calibrations as well as response calcs.

This interface can also read and write error terms from/to a Cal Set. However, ICalibrator is NOT recommended for this purpose. The [ICalSet2](#) Interface is better suited for reading and writing error terms.

See a vbscript example of [how to perform a 2-port Cal and read the cal data](#).

##### IGuidedCalibration

This interface provides the methods and properties used by the Guided Calibration wizard. With this interface you can perform multi-port calibrations (1 to 4 port calcs), but no response calcs.

##### ICalSet2 and ICalData3

These interfaces provide access to the Cal Set contents. You can read and write error terms with both of these interfaces.

- ICalSet2 uses Variant data, which means it is usable from vbscript.
- ICalData3 uses "typed" data, which means it can be used from any automation engine that can read the type library (VEE, VB, C++, etc.). Typed arguments (such as float or single) are more efficient than variants, so use the ICalData3 interface where better performance is needed.

See a vbscript example of [how to read Cal Set data](#).

##### ICalSet3

This interface provides access to the stimulus attributes of the Cal data: frequency, power, number of points. These are the stimulus conditions under which the Cal Set was created.

## Programming the PNA with C++

---

The programming information contained in this Help system is aimed at the Visual Basic programmer. VB does a lot of work for the programmer when it comes to managing and accessing components. Using a lower level language like C++ requires a more thorough understanding of the underlying tenets of COM. It is not the intent of this section to teach COM programming. The following is intended to acquaint you with some of the basic concepts you need to know in order to program against COM.

### [Initializing COM](#)

### [Importing the Type Library](#)

### [Creating the Application Object](#)

### [Errors](#)

### [Events](#)

### [Additional Reading](#)

### [Example](#)

---

**Note:** The information in this section assumes development on a Windows OS using Microsoft tools.

---

## Other Topics about COM Concepts

---


### Initializing COM

The first thing you must do before performing any COM transactions is to initialize the COM library. You can do this in a number of ways. The most basic of these is a call to **CoInitialize( )** or **CoInitializeEx( )**. Alternatively you can use the MFC (Microsoft Foundation Classes) **AfxOleInit( )**.

Conversely, before your program exits you must uninitialize COM. You can accomplish this with **CoUninitialize( )** or the MFC routine **AfxOleTerm( )**.

---

### Importing the Type Library

 To make a component available to the client, the server exports what is called the type library. For the PNA, this file is 835x.tlb. It is located on the PNA's hard drive at **C:\Program Files\Agilent\Network Analyzer\**

**Automation**. See [Configure for COM-DCOM Programming](#).

The type library can be read and deciphered using another COM interface called ITypeLib. VB uses this interface to present, for example, its object browser. Visual C++ can also read type libraries. This is done by importing the type library into your project with a compiler directive:

```
#import "C:\Program Files\Common Files\Agilent\Pna\835x.tlb", named_guids
```

When you compile your program with this statement in it, the compiler creates two other files: **835x.tlh** and **835x.tli**. The first is a header file that contains the type definitions for the PNA's COM interfaces and their methods. The second file contains inline functions that wrap the PNA's interface methods. The wrappers are beneficial in that they contain error reporting for each of the method calls.

The .tlh file defines a smart pointer which you can use to access the PNA's objects. The smart pointer definition looks like this:

```
_com_smartptr typedef(Iapplication, _uuidof(Iapplication))
```

A smart pointer is a term used for a C++ object that encapsulates a pointer used to refer to a COM object. All COM

objects derive from the interface IUnknown. This interface has three methods: QueryInterface( ), AddRef( ), and Release( ). The function of the AddRef and Release methods is to maintain a reference count on the object and thus control the object's lifetime. Anytime you copy or create a reference to a COM object, you are responsible for incrementing its reference count. And likewise, when you are finished using that reference, it is your responsibility to Release it. Smart pointers do this work for you, as shown in the [example program](#). In addition, smart pointers will also perform the QueryInterface call when required. QueryInterface is a method that requests a specific interface from an object. In the example program we gain access to the IArrayTransfer interface of the Measurement object. In the ReadMethod routine, we see this:

```
PTransferData = pMeas;
```

The assignment operator is overloaded for the smart pointer and in reality, this simple statement does this:

```
HRESULT hr = pMeas->QueryInterface(IID_IArrayTransfer, (void**)&pTransferData);
```

Using the existing interface pointer (pMeas) to the object, this call asks the object if it supports the IArrayTransfer interface, and if so to return a pointer to it in pTransferData. Smart pointer makes life easier for the C++ programmer. Read more about smart pointers in Microsoft Developer's Network Library (*MSDN*).

---

## Creating the Application Object

The only createable object exported by the PNA is the [Application object](#). Typically this would be done with a call to CoCreateInstance:

```
STDAPI CoCreateInstance(
 CLSID_IApplication, //Class identifier (CLSID) of the object
 NULL, //Pointer to controlling IUnknown
 CLSCTX_SERVER, //Context for running executable code
 IID_IApplication, //Reference to the IID of the interface
 (void**)&pNA //Address of output variable that receives
 // the interface pointer requested in riid
);
```

With the smart pointer, this is taken care of with the following call:

```
IApplicationPtr pNA; // declare the smart pointer
pNA = IApplicationPtr("AgilentPNA835x.Application.1");
```

---

## Errors

All COM method calls are required to return an HRESULT. This is 32 bit long with a specific format.

- The most significant bit indicates success(0) or failure(1).
- The lower 16 bits indicate the specific failure.

Visual Basic strips off the returned HRESULT and raises an error object for non-successful returns. The C++ programmer must himself be diligent about handling errors. You must check the return value of each COM call to ensure its success.

---

## Events

The Application object sources the INetworkAnalyzerEvents interface. This object is the source for all events. To use events in C++, you must do two things:

1. Implement the INetworkAnalyzerEvents interface - derive an object from INetworkAnalyzerEvents and implement the methods described there.
  2. Subscribe to the IconnectionPoint interface of the Application object. - obtain a pointer to the IconnectionPointContainer interface of the Application object and making the following request:
-

```
FindConnectionPoint(IID_INetworkAnalyzerEvents, &pConnection);
```

A successful call to this interface will return a valid pointer in pConnection. Use this pointer to subscribe to the Application object:

```
pConnect->Advise(IUnknown* punk, DWORD dwCookie);
```

This call provides the server object with a callback address. The IUnknown pointer in this call is the IUnknown pointer of the object that implements the INetworkAnalyzerEvents interface. This is the event sink. The application object needs a pointer to this object in order to call your interface when an event occurs. The **dwCookie** is your subscription key. Use it to unsubscribe (see Unadvise( ) ).

---

### Additional Reading

*"MSDN"* - Microsoft Developer's Network Library

*"Learning DCOM"*, by Thuan L. Thai, published by O'Reilly(1999)

*"Inside COM"*, by Dale Rogerson, published by Microsoft Press (1997)

*"Understanding ActiveX and OLE"*, by David Chappell, also published by Microsoft Press (1996)

*"Beginning ATL COM Programming"*, published by Wrox Press (1998)

---

### Example

The example uses the smart pointer created by Microsoft Visual Studio. The calls to CoInitialize and CoUninitialize open and close the COM libraries. In the example, notice that the pointers local to the main routine are explicitly released. When smart pointers go out of scope, they will perform this duty implicitly. However, we are calling CoUninitialize before they have the chance to be destroyed, so we are obliged to release them.

See the [example](#) program.

---

## Using COM from .NET

---

To communicate with the PNA from Microsoft .NET enabled languages such as C# and Visual Basic.NET perform the following steps:

1. Configure your PC and PNA for COM-DCOM Programming.
2. Reference the type library within the development environment (see the following exception for managed C++ projects.) In the process of referencing the type library, a .NET assembly is created that wraps the PNA type library with a .NET friendly interface. This .NET assembly is called an Interop Assembly.

To run a .NET program on the PNA, you will need to install the .NET framework on the PNA. This can be done by running the dotnetfx.exe program, located at: <http://www.microsoft.com/downloads/details.aspx?FamilyID=262d25e3-f589-4842-8157-034d1e7cf3a3&DisplayLang=en>

If you only intend to run .NET programs on a remote computer, then it is not necessary to install the .NET framework on the PNA."

**Exception for managed C++ projects:** To generate the Interop Assembly for managed C++ projects, you must use the tlbimp.exe utility. This utility is described in the MSDN documentation. On your PC, click Start then Run then type: tlbimp.exe 835x.tlb and click OK. After doing this you can use the #using directive to include the Interop Assembly on managed C++ projects.

### Registering the PNA Primary Interop Assembly (PIA) (OPTIONAL)

The PIA is NOT necessary to communicate with the PNA. The following procedure is useful only when there are two .NET programs that want to share the same PNA interface definitions. Without the PIA, each .NET application would use its own Interop Assembly.

To register the PIA on a machine, you need to have the common language runtime (CLR) installed. This is included with Visual Studio.NET. Then perform the following steps:

---

**Note:** In the following steps, replace <local directory> with the full path name of the specified file on your PC.

---

1. Run the PNAProxy.exe program as described in Configure for COM-DCOM Programming.
2. On the PNA, copy **C:\Program Files\Agilent\Network Analyzer\Automation\AgilentPNA835x.dll** to a local directory on your PC. Make a note of this directory.
3. On your PC, click **Start**, then **Run**, then type: **regasm <local directory> \AgilentPNA835x.dll** and click **OK** to register the dll.
4. Again, click **Start**, then **Run**, then type: **gacutil /i <local directory> \AgilentPNA835x.dll** and click **OK** to add the assembly to the Global Assembly Cache (GAC).

To **Uninstall the PIA**, perform the following:

1. On your PC, click **Start**, then **Run**, then type: **gacutil /u <local directory> \AgilentPNA835x.exe** and click **OK** to remove the assembly from the GAC.
2. On your PC, click **Start**, then **Run**, then type: **regasm /unregisiter <local directory> \ agilentpna835x.dll** and click **OK** to unregister the assembly.
3. To uninstall PNA Proxy.exe use the **Add/Remove Programs** utility in the control panel.





## List of PNA SCPI Commands

---

Click on a command for details

Local Lockout - GPIB Message

### COMMON COMMANDS

- \*CLS - Clear Status
- \*ESE - Event Status Enable
- \*ESE? - Event Status Enable Query
- \*ESR - Event Status Enable Register
- \*IDN? - Identify
- \*OPC - Operation complete command
- \*OPC? - Operation complete query
- \*OPT? - Identify Options Query
- \*RST - Reset
- \*SRE - Service Request Enable
- \*SRE? - Service Request Enable Query
- \*STB? - Status Byte Query
- \*TST? - Result of Self-test Query
- \*WAI - Wait

### ABORt Command

ABORt

### CALCulate:CORRection Commands

- CALCulate<ch>:CORRection:EDELay:MEDIum <num>
- CALCulate<ch>:CORRection:EDELay:TIME <num>
- CALCulate<ch>:CORRection:EDELay:WGCotoff <num>
- CALCulate<ch>:CORRection:[STATe] <on|off>
- CALCulate<ch>:CORRection:TYPE <char>
- CALCulate<ch>:CORRection:OFFSet[:MAGNitude] <num> OBSOLETE
- CALCulate<ch>:CORRection:OFFSet:PHASe <num>[<char>] OBSOLETE

### CALCulate:CUSTom Commands

- CALCulate<ch>:CUST:DEFine <Mname>, <ProgID> [,param]
- CALCulate<ch>:CUSTom:MODify <param>

### CALCulate:DATA Commands

- CALCulate<ch>:DATA <char>
- CALCulate<ch>:DATA:CUSTom <name>, <data>
- CALCulate<ch>:DATA:CUSTom:CATalog?
- CALCulate<ch>:DATA:SnP?

### CALCulate:FILTer Commands

- CALCulate<ch>:FILTer[:GATE]:COUPlE:PARAmeter <char>
- CALCulate<ch>:FILTer[:GATE]:TIME:CENTer <num>

CALCulate<ch>:FILTer[:GATE]:TIME:SHAPE <char>  
CALCulate<ch>:FILTer[:GATE]:TIME:SPAN <num>  
CALCulate<ch>:FILTer[:GATE]:TIME:STATE <boolean>  
CALCulate<ch>:FILTer[:GATE]:TIME:START <num>  
CALCulate<ch>:FILTer[:GATE]:TIME:STOP <num>  
CALCulate<ch>:FILTer[:GATE]:TIME[:TYPE] <char>

#### **CALCulate:FORMat Command**

CALCulate<ch>:FORMat <char>

#### **CALCulate:FSIMulator:BALun Commands**

CALCulate<ch>:FSIMulator:BALun:CZConversion:BPORT<pnum>:IMAG <value>  
CALCulate<ch>:FSIMulator:BALun:CZConversion:BPORT<pnum>:REAL <value>  
CALCulate<ch>:FSIMulator:BALun:CZConversion:BPORT<pnum>:Z0[:R] <value>  
CALCulate<ch>:FSIMulator:BALun:CZConversion:STATE <bool>  
CALCulate<ch>:FSIMulator:BALun:DEVICE <char>  
CALCulate<ch>:FSIMulator:BALun:DMCircuit:BPORT<pnum>:PARAMeters:C <value>  
CALCulate<ch>:FSIMulator:BALun:DMCircuit:BPORT<pnum>:PARAMeters:G <value>  
CALCulate<ch>:FSIMulator:BALun:DMCircuit:BPORT<pnum>:PARAMeters:L <value>  
CALCulate<ch>:FSIMulator:BALun:DMCircuit:BPORT<pnum>:PARAMeters:R <value>  
CALCulate<ch>:FSIMulator:BALun:DMCircuit:BPORT<pnum>[:TYPE] <char>  
CALCulate<ch>:FSIMulator:BALun:DMCircuit:BPORT<pnum>:USER:FILENAME <string>  
CALCulate<ch>:FSIMulator:BALun:DMCircuit:STATE <bool>  
CALCulate<ch>:FSIMulator:BALun:DZConversion:BPORT<pnum>:IMAG <value>  
CALCulate<ch>:FSIMulator:BALun:DZConversion:BPORT<pnum>:REAL <value>  
CALCulate<ch>:FSIMulator:BALun:DZConversion:BPORT<pnum>:Z0[:R] <value>  
CALCulate<ch>:FSIMulator:BALun:DZConversion:STATE <bool>  
CALCulate<ch>:FSIMulator:BALun:PARAMeter<n>:BBALanced[:DEFine] <char>  
CALCulate<ch>:FSIMulator:BALun:PARAMeter<n>:SBALanced[:DEFine] <char>  
CALCulate<ch>:FSIMulator:BALun:PARAMeter<n>:SSBalanced[:DEFine] <char>  
CALCulate<ch>:FSIMulator:BALun:PARAMeter<n>:STATE <bool>  
CALCulate<ch>:FSIMulator:BALun:TOPology:BBALanced[:PPORTs] <p1Pos>,<p1Neg>,<p2Pos>,<p2Neg>  
CALCulate<ch>:FSIMulator:BALun:TOPology:SBALanced[:PPORTs] <se>,<bPos>,<bNeg>  
CALCulate<ch>:FSIMulator:BALun:TOPology:SSBalanced[:PPORTs] <se1>,<se2>,<bPos>,<bNeg>

#### **CALCulate:FSIMulator:EMBed Commands**

CALCulate<ch>:FSIMulator:EMBed:NETWork<n>:FILENAME <string>  
CALCulate<ch>:FSIMulator:EMBed:NETWork<n>:TYPE <char>  
CALCulate<ch>:FSIMulator:EMBed:STATE <bool>  
CALCulate<ch>:FSIMulator:EMBed:TOPology:A:PORTs <p1>,<p2>  
CALCulate<ch>:FSIMulator:EMBed:TOPology:B:PORTs <p1>,<p2>,<p3>  
CALCulate<ch>:FSIMulator:EMBed:TOPology:C:PORTs <p1>,<p2>,<p3>,<p4>

CALCulate<ch>:FSIMulator:EMBed:TYPE <char>

### **CALCulate:FSIMulator:SENDED Commands**

CALCulate<ch>:FSIMulator:SENDED:DEEMbed:PORT<n>[:TYPE] <char>  
CALCulate<ch>:FSIMulator:SENDED:DEEMbed:PORT<n>:USER:FILENAME <string>  
CALCulate<ch>:FSIMulator:SENDED:DEEMbed:PORT<n>:STATE <bool>  
CALCulate<ch>:FSIMulator:SENDED:PMcircuit:PORT<n>:PARAmeters:C <value>  
CALCulate<ch>:FSIMulator:SENDED:PMcircuit:PORT<n>:PARAmeters:G <value>  
CALCulate<ch>:FSIMulator:SENDED:PMcircuit:PORT<n>:PARAmeters:L <value>  
CALCulate<ch>:FSIMulator:SENDED:PMcircuit:PORT<n>:PARAmeters:R <value>  
CALCulate<ch>:FSIMulator:SENDED:PMcircuit:PORT<n>[:TYPE] <char>  
CALCulate<ch>:FSIMulator:SENDED:PMcircuit:PORT<n>:USER:FILENAME <string>  
CALCulate<ch>:FSIMulator:SENDED:PMcircuit:STATE <bool>  
CALCulate<ch>:FSIMulator:SENDED:ZCONversion:PORT<n>:IMAG <value>  
CALCulate<ch>:FSIMulator:SENDED:ZCONversion:PORT<n>:REAL <value>  
CALCulate<ch>:FSIMulator:SENDED:ZCONversion:PORT<n>:ZO[:R] <value>  
CALCulate<ch>:FSIMulator:SENDED:ZCONversion:STATE <bool>  
CALCulate<ch>:FSIMulator:STATE <bool>

### **CALCulate:FUNCTION Commands**

CALCulate<ch>:FUNCTION:DATA?  
CALCulate<ch>:FUNCTION:DOMain:USER[:RANGE] <range>  
CALCulate<ch>:FUNCTION:DOMain:USER:START <range>, <start>  
CALCulate<ch>:FUNCTION:DOMain:USER:STOP <range>, <stop>  
CALCulate<ch>:FUNCTION:EXECute  
CALCulate<ch>:FUNCTION:STATistics[:STATE] <ON|OFF>  
CALCulate<ch>:FUNCTION:TYPE <char>

### **CALCulate:LIMIT Commands**

CALCulate<ch>:LIMit:DATA <block>  
CALCulate<ch>:LIMit:DISPlay[:STATE] <ON | OFF>  
CALCulate<ch>:LIMit:SEGMENT<snum>AMPLitude:START <num>  
CALCulate<ch>:LIMit:SEGMENT<snum>AMPLitude:STOP <num>  
CALCulate<ch>:LIMit:SEGMENT<snum>STIMulus:START <num>  
CALCulate<ch>:LIMit:SEGMENT<snum>STIMulus:STOP <num>  
CALCulate<ch>:LIMit:SEGMENT<snum>:TYPE <char>  
CALCulate<ch>:LIMit:SOUND[:STATE] <ON | OFF>  
CALCulate<ch>:LIMit:STATE <ON | OFF>

### **CALCulate:MARKer Commands**

CALCulate<ch>:MARKer:AOff  
CALCulate<ch>:MARKer:BWIDth <num>  
CALCulate<ch>:MARKer<mkr>:COUPLing[:STATE] <ON|OFF>  
CALCulate<ch>:MARKer<mkr>:DELTA <ON|OFF>  
CALCulate<ch>:MARKer<mkr>:DIScrete <ON|OFF>  
CALCulate<ch>:MARKer<mkr>:DISTance <num>

CALCulate<ch>:MARKer<mkr>:FORMat <char>  
 CALCulate<ch>:MARKer<mkr>:FUNction:APEak:EXCursion <num>  
 CALCulate<ch>:MARKer<mkr>:FUNction:APEak:THReshold <num>  
 CALCulate<ch>:MARKer<mkr>:FUNction:DOMain:USER <range>  
 CALCulate<ch>:MARKer<mkr>:FUNction:DOMain:USER:STARt <start>  
 CALCulate<ch>:MARKer<mkr>:FUNction:DOMain:USER:STOP <stop>  
 CALCulate<ch>:MARKer<mkr>:FUNction:EXECute [<func>]  
 CALCulate<ch>:MARKer<mkr>:FUNction[:SElect] <char>  
 CALCulate<ch>:MARKer<mkr>:TARGet <num>  
 CALCulate<ch>:MARKer<mkr>:FUNction:TRACking <ON | OFF>  
 CALCulate<ch>:MARKer:REFerence[:STATe] <ON | OFF>  
 CALCulate<ch>:MARKer:REFerence:X <num>  
 CALCulate<ch>:MARKer:REFerence:Y?  
 CALCulate<ch>:MARKer<mkr>:TYPE <char>  
 CALCulate<ch>:MARKer<mkr>:SET <char>  
 CALCulate<ch>:MARKer<mkr>[:STATe] <ON|OFF>  
 CALCulate<ch>:MARKer<mkr>:X <num>  
 CALCulate<ch>:MARKer<mkr>:Y?

#### **CALCulate:MATH Commands**

CALCulate<ch>:MATH:FUNction <char>  
 CALCulate<ch>:MATH:MEMorize

#### **CALCulate:MIXer Command**

CALCulate<ch>:MIXer:XAXis <char>

#### **CALCulate:NORMalize Commands**

CALCulate<ch>:NORMalize[:IMMediate] OBSOLETE  
 CALCulate<ch>:NORMalize:STATe <ON | OFF> OBSOLETE  
 CALCulate<ch>:NORMalize:INTerpolation[:STATe] <ON | OFF> OBSOLETE

#### **CALCulate:OFFSet Commands**

CALCulate<ch>:OFFSet:MAGNitude <num>  
 CALCulate<ch>:OFFSet:MAGNitude:SLOPe <num>  
 CALCulate<ch>:OFFSet:PHASe <num>[<char>]

#### **CALCulate:PARAmeter Commands**

CALCulate<ch>:PARAmeter:CATalog?  
 CALCulate<ch>:PARAmeter:DEFine <Mname>,<param>[,load]  
 CALCulate<ch>:PARAmeter:DELete <Mname>  
 CALCulate:PARAmeter:DELete:ALL  
 CALCulate<ch>:PARAmeter:MNUMBER?  
 CALCulate<ch>:PARAmeter::MODify <param>  
 CALCulate<ch>:PARAmeter:SElect <Mname>

#### **CALCulate:RDATa Commands**

CALCulate<ch>:RDATa? <char>

### **CALCulate:SMOothing Commands**

CALCulate<ch>:SMOothing:APERture <num>  
CALCulate<ch>:SMOothing:POINts <num>  
CALCulate<ch>:SMOothing[:STATe] <ON | OFF>

### **CALCulate:TRANSform Commands**

CALCulate<ch>:TRANSform:COUPlE:PARAmeters <num>  
CALCulate<ch>:TRANSform:TIME:CENTer <num>  
CALCulate<ch>:TRANSform:TIME:IMPulse:WIDTh <num>  
CALCulate<ch>:TRANSform:TIME:KBESsel <num>  
CALCulate<ch>:TRANSform:TIME:LPFREQuency  
CALCulate<ch>:TRANSform:TIME:MARKer:MODE <char>  
CALCulate<ch>:TRANSform:TIME:MARKer:UNIT <char>  
CALCulate<ch>:TRANSform:TIME:SPAN <num>  
CALCulate<ch>:TRANSform:TIME:STARt <num>  
CALCulate<ch>:TRANSform:TIME:STATe <ON | OFF>  
CALCulate<ch>:TRANSform:TIME:STOP <num>  
CALCulate<ch>:TRANSform:TIME:STEP:RTIME <num>  
CALCulate<ch>:TRANSform:TIME:STIMulus <char>  
CALCulate<ch>:TRANSform:TIME[:TYPE] <char>

### **CONTRol:AUXiliary Commands**

CONTRol:AUXiliary:C[:DATA] <num>  
CONTRol:AUXiliary:C:LOGic <char>  
CONTRol:AUXiliary:C:MODE <char>  
CONTRol:AUXiliary:FOOTswitch?  
CONTRol:AUXiliary:FOOTswitch:MODE <char>  
CONTRol:AUXiliary:INPut:VOLTage?  
CONTRol:AUXiliary:OUTPut<out>:MODE <char>  
CONTRol:AUXiliary:OUTPut<out>:Voltage <num>  
CONTRol:AUXiliary:PASSfail:LOGic <char>  
CONTRol:AUXiliary:PASSfail:MODE <char>  
CONTRol:AUXiliary:PASSfail:SCOPE <char>  
CONTRol:AUXiliary:SWEepend <char>

### **CONTRol:EXTernal:TESTSet Commands**

CONTRol:EXTernal:TESTset:DATa <addr>,<data>  
CONTRol:EXTernal:TESTset:INTerrupt?  
CONTRol:EXTernal:TESTset:RAWData <data>  
CONTRol:EXTernal:TESTset:SWEepholdoff?

### **CONTRol:HANDler Commands**

CONTRol:HANDler:C:MODE <char>  
CONTRol:HANDler:D:MODE <char>  
CONTRol:HANDler:<port>[:DATa] <num>

CONTRol:HANDler:INPut?  
CONTRol:HANDler:LOGic <char>  
CONTRol:HANDler:OUTPut<num>[:DATa] <num2>  
CONTRol:HANDler:OUTPut<num>:USER[:DATa] <num2>  
CONTRol:HANDler:PASSfail:LOGic <char>  
CONTRol:HANDler:PASSfail:MODE <char>  
CONTRol:HANDler:PASSfail:SCOPE <char>  
CONTRol:HANDler:PASSfail:POLicy  
CONTRol:HANDler:PASSfail:STATus?  
CONTRol:HANDler:SWEepend <char>

### **CONTRol:SIGNal Commands**

CONTRol:SIGNal <conn>,<char>  
CONTRol:SIGNal:TRIGger:ATBA <bool>  
CONTRol:SIGNal:TRIGger:OUTP <bool>

### **DISPLay Commands**

DISPLay:ANNotation:FREQuency[:STATe] <ON | OFF>  
DISPLay:ANNotation:MESSAge:STATe <ON | OFF>  
DISPLay:ANNotation:STATus <ON|OFF>  
DISPLay:ARRange <char>  
DISPLay:CATalog?  
DISPLay:ENABLE <ON | OFF>  
DISPLay:FSIGN <ON | OFF>  
DISPLay[:TILE] OBSOLETE  
DISPLay:WINDow<wnum>:ANNotation:MARKer:SINGle[:STATe] <bool>  
DISPLay:WINDow<wnum>:ANNotation:MARKer:SIZE <char>  
DISPLay:WINDow<wnum>:ANNotation:MARKer:STATe <ON|OFF>  
DISPLay:WINDow<wnum>:ANNotation:TRACe:STATe <ON|OFF>  
DISPLay:WINDow<wnum>:CATalog?  
DISPLay:WINDow<wnum>:ENABLE <ON | OFF>  
DISPLay:WINDow<wnum>:SIZE MIN | MAX | NORM  
DISPLay:WINDow<wnum>[:STATe] <ON | OFF>  
DISPLay:WINDow<wnum>:TABLe <char>  
DISPLay:WINDow<wnum>:TITLe:DATA <string>  
DISPLay:WINDow<wnum>:TITLe[:STATe] <ON | OFF>  
DISPLay:WINDow<wnum>:TRACe<tnum>:DELeTe  
DISPLay:WINDow<wnum>:TRACe<tnum>:FEED <name>  
DISPLay:WINDow<wnum>:TRACe<tnum>MEMory[:STATe] <ON | OFF>  
DISPLay:WINDow<wnum>:TRACe<tnum>:SELect  
DISPLay:WINDow<wnum>:TRACe<tnum>[:STATe] <ON | OFF>  
DISPLay:WINDow<wnum>:TRACe<tnum>:Y[:SCALE]:AUTO  
DISPLay:WINDow<wnum>:TRACe<tnum>:Y[:SCALE]:PDIVision <num>  
DISPLay:WINDow<wnum>:TRACe<tnum>:Y[:SCALE]:RLEVel <num>  
DISPLay:WINDow<wnum>:TRACe<tnum>:Y[:SCALE]:RPOSition <num>

## **FORMat Commands**

FORMat:BORDER <char>

FORMat[:DATA] <char>

## **HARDcopy Command**

HCOPY:FILE

HCOPY[:IMMEDIATE]

## **INITiate Commands**

INITiate:CONTInuous <boolean>

INITiate<ch>[:IMMEDIATE]

## **MMEMory Commands**

MMEMory:CATalog[:<char>]? [<folder>]

MMEMory:CDIRectory <folder>

MMEMory:COPY <file1>,<file2>

MMEMory:DELeTe <file>

MMEMory:LOAD[:<char>] <file>

MMEMory:MDIRectory <folder>

MMEMory:MOVE <file1>,<file2>

MMEMory:RDIRectory <folder>

MMEMory:STORe[:<char>] <file>

MMEMory:STORe:CIT:DATA <filename>

MMEMory:STORe:CIT:FORMat <filename>

MMEMory:STORe:TRACe:CONTents:CITifile <char>

MMEMory:STORe:TRACe:FORMat:CITifile <char>

MMEMory:STORe:TRACe:FORMat:SNP <char>

MMEMory:TRANsfer <fileName>,<dataBlock>

## **OUTPut Command**

OUTPut[:STATe] <ON | OFF>

## **SENSe:AVERage Commands**

SENSe<ch>:AVERage:CLear

SENSe<ch>:AVERage:COUNt <num>

SENSe<ch>:AVERage[:STATe] <ON | OFF>

## **SENSe:BANDwidth Command**

SENSe<ch>:BANDwidth | BWIDth[:RESolution] <num>

SENSe<ch>:BANDwidth | BWIDth:TRACk <bool>

## **SENSe:CORRection Commands**

SENSe<ch>:CORRection:CHeck[:ACQuire] <char>

SENSe<ch>:CORRection:CHeck:DONE

SENSe<ch>:CORRection:CHeck:PARAmeter <Mname>

SENSe<ch>:CORRection:COLLect[:ACQuire] <class>[,sub]

SENSe<ch>:CORRection:COLLect:APPLY



SENSE<ch>:CORRection:COLLect:MEthod <char>  
 SENSE<ch>:CORRection:COLLect:SAVE  
 SENSE:CORRection:IMPedance:INPut:MAGNitude <num>  
 SENSE<ch>:CORRection:INTerpolation[:STATe] <ON | OFF>  
 SENSE<ch>:CORRection:ISOLation[:STATe] <ON | OFF> OBSOLETE  
 SENSE:CORRection:PREFerence:CSET:SAVUser  
 SENSE:CORRection:PREFerences:ECAL:ORientation[:STATe] <ON|OFF>  
 SENSE:CORRection:PREFerences:ECAL:PMAP <module>,<string>  
 SENSE<ch>:CORRection:RVELocity:COAX <num>  
 SENSE:CORRection:SFORward[:STATe] <boolean>  
 SENSE<ch>:CORRection[:STATe] <ON | OFF>  
 SENSE:CORRection:TSTandards[:STATe] <boolean>  
 SENSE:CORRection:TYPE:CATalog? <char>

**SENSe:CORRection:CKIT Commands**

SENSE<ch>:CORRection:CKIT:CLEar[:IMMEDIATE]  
 SENSE<ch>:CORRection:CKIT:COUNt?  
 SENSE<ch>:CORRection:CKIT:IMPort <string>  
 SENSE<ch>:CORRection:CKIT:INITialize[:IMMEDIATE]  
 SENSE<ch>:CORRection:CKIT:LOAD <string>

**SENSe:CORRection:COLLect:CKIT Commands**

SENSE:CORRection:COLLect:CKIT:CONNector:ADD <family>,<start>,<stop>,<z0>,<gender>,<media>,<cutoff>  
 SENSE:CORRection:COLLect:CKIT:CONNector:CATalog?  
 SENSE:CORRection:COLLect:CKIT:CONNector:DELeTe  
 SENSE:CORRection:COLLect:CKIT:CONNector:FNAME <name>  
 SENSE:CORRection:COLLect:CKIT:CONNector:SNAME <family>,<gender>,<port>  
 SENSE:CORRection:COLLect:CKIT:DESCRiption <string>  
 SENSE:CORRection:COLLect:CKIT:INFORMATION? <module>[,char]  
 SENSE:CORRection:COLLect:CKIT:NAME <name>  
 SENSE:CORRection:COLLect:CKIT:OLIST[class]?  
 SENSE:CORRection:COLLect:CKIT:ORDeR<class> <std> [,<std>] [,<std>] [,<std>] [,<std>] [,<std>] [,<std>]  
 SENSE:CORRection:COLLect:CKIT:RESet <num>  
 SENSE:CORRection:COLLect:CKIT[:SELeCt] <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:C0 <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:C1 <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:C2 <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:C3 <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:CHARacter <char>  
 SENSE:CORRection:COLLect:CKIT:STANdard:DELay <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:FMAX <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:FMIN <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:IMPedance <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:L0 <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:L1 <num>  
 SENSE:CORRection:COLLect:CKIT:STANdard:L2 <num>

SENSE:CORRection:COLLect:CKIT:STANdard:L3 <num>  
SENSE:CORRection:COLLect:CKIT:STANdard:LABel <name>  
SENSE:CORRection:COLLect:CKIT:STANdard:LOSS <num>  
SENSE:CORRection:COLLect:CKIT:STANdard:REMOve  
SENSE:CORRection:COLLect:CKIT:STANdard:SDEsCription <string>  
SENSE:CORRection:COLLect:CKIT:STANdard[:SELEct] <num>  
SENSE:CORRection:COLLect:CKIT:STANdard:TYPE <char>

#### **SENSE:CORRection:CSET Commands**

SENSE:CORRection:CSET:CATalog?  
SENSE<ch>:CORRection:CSET:CREate  
SENSE<ch>:CORRection:CSET:DATA  
SENSE<ch>:CORRection:CSET:DELEte <string>  
SENSE<ch>:CORRection:CSET:DESCRiption <string>  
SENSE<ch>:CORRection:CSET:GUID <string>  
SENSE<ch>:CORRection:CSET:NAME  
SENSE<ch>:CORRection:CSET[:SELEct] <char>  
SENSE<ch>:CORRection:CSET:SAVE <char>

#### **SENSE:CORRection:COLLect:GUIDed Commands**

SENSE:CORRection:COLLect:GUIDed:ACQuire <std>  
SENSE:CORRection:COLLect:GUIDed:CKIT:PORT<pnum>:CATalog?  
SENSE:CORRection:COLLect:GUIDed:CKIT:PORT<pnum>[:SELEct] <kit>  
SENSE:CORRection:COLLect:GUIDed:CONNector:CATalog?  
SENSE:CORRection:COLLect:GUIDed:CONNector:PORT<pnum>[:SELEct] <conn>  
SENSE:CORRection:COLLect:GUIDed:DESCRiption? <step>  
SENSE:CORRection:COLLect:GUIDed:DMATch[:INITiate] <port1Conn>,<cKit>  
SENSE:CORRection:COLLect:GUIDed:DMATch:APPLY:PORTs?  
SENSE:CORRection:COLLect:GUIDed:DMATch:APPLY[:IMMediate] [<CalSetGUID>]  
SENSE<ch>:CORRection:COLLect:GUIDed:INITiate  
SENSE:CORRection:COLLect:GUIDed:METHod  
SENSE:CORRection:COLLect:GUIDed:SAVE  
SENSE:CORRection:COLLect:GUIDed:STEPs?

#### **SENSE:CORRection:COLLect:SESSion:Commands**

SENSE<ch>:CORRection:COLLect:SESSion<n>:ACQuire <step>  
SENSE<ch>:CORRection:COLLect:SESSion<n>:CKIT:PORT<pnum>:CATalog?  
SENSE<ch>:CORRection:COLLect:SESSion<n>:CKIT:PORT<pnum>[:SELEct] <kit>  
SENSE<ch>:CORRection:COLLect:SESSion<n>:CONNector:PORT<pnum>[:SELEct] <conn>  
SENSE<ch>:CORRection:COLLect:SESSion<n>:DESCRiption? <step>  
SENSE<ch>:CORRection:COLLect:SESSion<n>:INITiate<string>  
SENSE<ch>:CORRection:COLLect:SESSion<n>:DONE  
SENSE<ch>:CORRection:COLLect:SESSion<n>:SAVE?  
SENSE<ch>:CORRection:COLLect:SESSion<n>:STEPs?

#### **SENSE:CORRection:COLLect:SESSion:SMC Commands**

SENSe<ch>:CORRection:COLLEct:SESSion<n>:SMC:ECAL:CHARacteriza <mod> ,<char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:SMC:PWRCal:SRCPort <char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:SMC:TWOPort:ECAL:ORlentation[:STATe] <bool>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:SMC:TWOPort:ECAL:PORTmap <mod> , <string>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:SMC:TWOPort:METhod <char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:SMC:TWOPort:OMITisolat <bool>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:SMC:TWOPort:OPTion <char>

#### **SENSe:CORRection:COLLEct:SESSion:VMC Commands**

SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:CHARacterize:CAL:FILEname <string>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:MIXer:CHARacterize:CAL: OPTion <char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:MIXer:CHARacterize:CAL: REVERSE <bool>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:MIXer:ECAL:CHARacteriza <mod> ,<char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:MIXer:ECAL:PORTmap <mod> , <string>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:OPERation <char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:TWOPort:ECAL:CHARacteriza <mod> ,<char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:TWOPort:ECAL:ORlentation[:STATe] <bool>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:TWOPort:ECAL:PORTmap <mod> , <string>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:TWOPort:METhod <char>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:TWOPort:OMITisolat <bool>  
SENSe<ch>:CORRection:COLLEct:SESSion<n>:VMC:TWOPort:OPTion <char>

#### **SENSe:CORRection:EXTension Commands**

SENSe<ch>:CORRection:EXTension:AUTO:CONFIg <char>  
SENSe<ch>:CORRection:EXTension:AUTO:LOSS <bool>  
SENSe<ch>:CORRection:EXTension:AUTO:MEASure <char>  
SENSe<ch>:CORRection:EXTension:AUTO:PORT<n> <bool>  
SENSe<ch>:CORRection:EXTension:AUTO:RESet  
SENSe<ch>:CORRection:EXTension:AUTO:STARt <value>  
SENSe<ch>:CORRection:EXTension:AUTO:STOP <value>  
SENSe<ch>:CORRection:EXTension:PORT<pnum>:FREQ<n> <value>  
SENSe<ch>:CORRection:EXTension:PORT<pnum>:INCLude<n>:STATe <bool>  
SENSe<ch>:CORRection:EXTension:PORT<pnum>:LDC <value>  
SENSe<ch>:CORRection:EXTension:PORT<pnum>:LOSS<n> <value>  
SENSe<ch>:CORRection:EXTension:PORT<pnum>[:TIME] <num>  
SENSe<ch>:CORRection:EXTension:RECeiver<Rnum>[:TIME] <num> OBSOLETE  
SENSe<ch>:CORRection:EXTension[:STATe] <ON | OFF>

#### **SENSe:COUPlE Commands**

SENSe<ch>:COUPlE <ALL | NONE>  
SENSe<ch>:COUPlE:PARAmeter

#### **SENSe:FREQUency Commands**

SENSe<ch>:FREQUency:CENTer <num>  
SENSe<ch>:FREQUency[:CW |:FIXed] <num>

SENSe<ch>:FREQUency:SPAN <num>  
SENSe<ch>:FREQUency:START <num>  
SENSe<ch>:FREQUency:STOP <num>

### **SENSe:IF Commands**

SENSe<ch>:IF:FILTer:SAMPlE:COUNt <num>  
SENSe<ch>:IF:FILTer:SAMPlE:COUNt:MODE <char>  
SENSe<ch>:IF:FILTer:SAMPlE:PERiod <num>  
SENSe<ch>:IF:FILTer:SAMPlE:PERiod:CATalog?  
SENSe<ch>:IF:FILTer:SAMPlE:PERiod:MODE <char>  
SENSe<ch>:IF:GAIN:ALL[:STATe] <char>  
SENSe<ch>:IF:GAIN:LEVel <id>, <level>  
SENSe<ch>:IF:GAIN[:STATe]?, <id>  
SENSe<ch>:IF:GATE:STATe <boolean>  
SENSe<ch>:IF:SOURce:PATH <id>, <char>

### **SENSe:MIXer Commands**

SENSe<ch>:MIXer:APPLy  
SENSe<ch>:MIXer:AVOIdspurs <bool>  
SENSe<ch>:MIXer:CALCulate <char>  
SENSe<ch>:MIXer:IF:FREQUency:DENominator <value>  
SENSe<ch>:MIXer:IF:FREQUency:FIXed <value>  
SENSe<ch>:MIXer:IF:FREQUency:NUMerator <value>  
SENSe<ch>:MIXer:IF:FREQUency:SIDeband <value>  
SENSe<ch>:MIXer:IF:FREQUency:START <value>  
SENSe<ch>:MIXer:IF:FREQUency:STOP <value>  
SENSe<ch>:MIXer:INPut:FREQUency:DENominator <value>  
SENSe<ch>:MIXer:INPut:FREQUency:FIXed<value>  
SENSe<ch>:MIXer:INPut:FREQUency:NUMerator <value>  
SENSe<ch>:MIXer:INPut:FREQUency:START <value>  
SENSe<ch>:MIXer:INPut:FREQUency:STOP <value>  
SENSe<ch>:MIXer:INPut:POWer <value>  
SENSe<ch>:MIXer:LO<n>:FREQUency:DENominator <value>  
SENSe<ch>:MIXer:LO<n>:FREQUency:FIXed <value>  
SENSe<ch>:MIXer:LO<n>:FREQUency:ILTI <value>  
SENSe<ch>:MIXer:LO<n>:FREQUency:MODE <char>  
SENSe<ch>:MIXer:LO<n>:FREQUency:NUMerator <value>  
SENSe<ch>:MIXer:LO<n>:NAME <value>  
SENSe<ch>:MIXer:LO<n>:POWer <value>  
SENSe<ch>:MIXer:LOAD <name>  
SENSe<ch>:MIXer:OUTput:FREQUency:SIDeband <value>  
SENSe<ch>:MIXer:OUTput:FREQUency:START <value>  
SENSe<ch>:MIXer:OUTput:FREQUency:STOP <value>  
SENSe<ch>:MIXer:SAVE <name>

SENSe<ch>:MIXer:STAGe <n>

### **SENSe:MUlTIpLexer Commands**

SENSe<ch>:MUlTIpLexer<id>:COUNt?

SENSe<ch>:MUlTIpLexer<id>:DISPlay[:STATe] <bool>

SENSe<ch>:MUlTIpLexer<id>:TSET:OUTPut[:DATA] <data>

SENSe<ch>:MUlTIpLexer<id>:TSET9:PORT1 <char>

SENSe<ch>:MUlTIpLexer<id>:TSET9:PORT2 <char>

SENSe<ch>:MUlTIpLexer<id>:TSET9:PORT3 <char>

SENSe<ch>:MUlTIpLexer<id>:TSET9:PORT4 <char>

SENSe<ch>:MUlTIpLexer<id>:STATe <bool>

### **SENSe:OFFSet Commands**

SENSe<ch>:OFFSet:CW <bool>

SENSe<ch>:OFFSet:DIVisor <num>

SENSe<ch>:OFFSet:MUlTIpLier <num>

SENSe<ch>:OFFSet:OFFSet <num>

SENSe<ch>:OFFSet:STARt?

SENSe<ch>:OFFSet[:STATe] <bool>

SENSe<ch>:OFFSet:STOP?

### **SENSe:POWer Command**

SENSe<ch>:POWer:ATTenuation <recvr>,<num>

### **SENSe:ROSCillator Command**

SENSe:ROSCillator:SOURce?

### **SENSe:SEGMENT Commands**

SENSe<ch>:SEGMENT<snum>:ADD

SENSe<ch>:SEGMENT:ARBITrary

SENSe<ch>:SEGMENT<snum>:BWIDth[:RESolution] <num>

SENSe<ch>:SEGMENT:BWIDth[:RESolution]:CONTRol <ON | OFF>

SENSe<ch>:SEGMENT:COUNt?

SENSe<ch>:SEGMENT<snum>:DELete

SENSe<ch>:SEGMENT:DELete:ALL

SENSe<ch>:SEGMENT<snum>:FREQUency:CENTer <num>

SENSe<ch>:SEGMENT<snum>:FREQUency:SPAN <num>

SENSe<ch>:SEGMENT<snum>:FREQUency:START <num>

SENSe<ch>:SEGMENT<snum>:FREQUency:STOP <num>

SENSe<ch>:SEGMENT<snum>:POWer[<port>][:LEVel] <num>

SENSe<ch>:SEGMENT:POWer[:LEVel]:CONTRol <ON | OFF>

SENSe<ch>:SEGMENT<snum>[:STATe] <ON | OFF>

SENSe<ch>:SEGMENT<snum>:SWEep:POINts <num>

SENSe<ch>:SEGMENT<snum>:SWEep:TIME <num>

SENSe<ch>:SEGMENT:SWEEp:TIME:CONTRol <ON | OFF>

## **SENSe:SWEEp Commands**

SENSe<ch>:SWEEp:DWELl <num>  
SENSe<ch>:SWEEp:DWELl:AUTO <ON | OFF>  
SENSe<ch>:SWEEp:GENeration <char>  
SENSe<ch>:SWEEp:GRoups:COUNt <num>  
SENSe<ch>:SWEEp:MODE <char>  
SENSe<ch>:SWEEp:POINts <num>  
SENSe<ch>:SWEEp:SRCPort <1 | 2>  
SENSe<ch>:SWEEp:TIME <num>  
SENSe<ch>:SWEEp:TIME:AUTO <ON | OFF>  
SENSe<ch>:SWEEp:TRIGger:DELay <num>  
SENSe<ch>:SWEEp:TRIGger:POINt <ON | OFF>  
SENSe<ch>:SWEEp:TYPE <char>

## **SENSe:X: Command**

SENSe<ch>:X:VALues?

## **SOURce Commands**

SOURce<ch>:POWer<port>:ATTenuation <num>  
SOURce<ch>:POWer<port>:ATTenuation:AUTO <ON | OFF>  
SOURce<ch>:POWer:CENTer <num>  
SOURce<ch>:POWer:COUPle <ON | OFF>  
SOURce<ch>:POWer:DETector <INTernal | EXTernal>  
SOURce<ch>:POWer<port>[:LEVel][:IMMediate] [:AMPLitude] <num>  
SOURce<ch>:POWer[:LEVel]:SLOPe <int>  
SOURce<ch>:POWer[:LEVel]:SLOPe:STATe <ON|OFF>  
SOURce<ch>:POWer:SPAN <num>  
SOURce<ch>:POWer:STARt <num>  
SOURce<ch>:POWer:STOP <num>

## **SOURce:POWer:CORRection Commands**

SOURce<ch>:POWer<port>:CORRection:COLLect:ABORt  
SOURce<ch>:POWer<port>:CORRection:COLLect[:ACQuire] <char>  
SOURce<ch>:POWer<port>:CORRection:COLLect:AVERage[:COUNt] <num>  
SOURce<ch>:POWer<port>:CORRection:COLLect:AVERage:NTOLerance <num>  
SOURce<ch>:POWer:CORRection:COLLect:DISPlay[:STATe] <ON | OFF>  
SOURce<ch>:POWer:CORRection:COLLect:FCHeck[:STATe] <ON | OFF>  
SOURce<ch>:POWer<port>:CORRection:COLLect:ITERation[:COUNt] <num>  
SOURce<ch>:POWer<port>:CORRection:COLLect:ITERation:TOLerance <num>  
SOURce<ch>:POWer<port>:CORRection:COLLect:METhod <char>  
SOURce<ch>:POWer<port>:CORRection:COLLect:SAVE  
SOURce<ch>:POWer:CORRection:COLLect:<pmChan>SENsor[:FRANge] <num1>,<num2>  
SOURce<ch>:POWer:CORRection:COLLect:<pmChan>SENsor:RCFactor <num>  
SOURce<ch>:POWer:CORRection:COLLect:<pmChan>SENsor:SELect  
SOURce<ch>:POWer:CORRection:COLLect:TABLE:DATA <data>

SOURce<ch>:POWER:CORRection:COLLect:TABLE:FREQUency <data>  
SOURce<ch>:POWER:CORRection:COLLect:TABLE:LOSS[:STATe] <ON | OFF>  
SOURce<ch>:POWER:CORRection:COLLect:TABLE:POINts?  
SOURce<ch>:POWER:CORRection:COLLect:TABLE[:SElect] <char>  
SOURce<ch>:POWER<port>:CORRection:DATA <data>  
SOURce<ch>:POWER<port>:CORRection:LEVel <num>  
SOURce<ch>:POWER<port>:CORRection:OFFSet[:MAGNitude] <num>  
SOURce<ch>:POWER<port>:CORRection[:STATe] <ON|OFF>

### **STATus REGISTER Commands**

Status Byte Register Commands  
STATus:QUEStionable:<keyword>  
STATus:QUEStionable:INTegrity <keyword>  
STATus:QUEStionable:INTegrity:HARDWare<keyword>  
STATus:QUEStionable:INTegrity:MEASurement<n> <keyword>  
STATus:QUEStionable:LIMit<n> <keyword>  
STATus:QUEStionable:DEFine<keyword>  
STATus:QUEStionable:DEFine:USER<1|2|3><keyword>  
Standard Event Status Register Commands  
STATus:OPERation<keyword>  
STATus:OPERation:AVERaging<n> <keyword>  
STATus:OPERation:DEFine<keyword>  
STATus:OPERation:DEFine:USER<1|2|3><keyword>

### **SYSTem Commands**

SYSTem:CHANnels:HOLD  
SYSTem:CHANnels:RESume  
SYSTem:COMMunicate:GPIB:RDEVice:CLOSe <ID>  
SYSTem:COMMunicate:GPIB:RDEVice:OPEN <bus>, <addr>, <timeout>  
SYSTem:COMMunicate:GPIB:RDEVice:READ? <ID>  
SYSTem:COMMunicate:GPIB:RDEVice:RESet  
SYSTem:COMMunicate:GPIB:RDEVice:WRITe <ID>,<string>  
SYSTem:COMMunicate:GPIB:PMETer:ADDRes <num>  
SYSTem:CORRection:WIZard <char>  
SYSTem:ERRor?  
SYSTem:ERRor:COUNt?  
SYSTem:FPReset  
SYSTem:MACRo:CoPY:CHANnel  
SYSTem:PRESet  
SYSTem:SECurity[:LEVel]  
SYSTem:UPReset  
SYSTem:UPReset:FPANel[:STATe] <bool>  
SYSTem:UPReset:LOAD <file>  
SYSTem:UPReset:SAVE[:STATe]

### **TRIGger Commands**

TRIGger:DElAy<num>

TRIGger[:SEQuence]:LEVel <char> OBSOLETE

TRIGger[:SEQuence]:SCOPE <char>

TRIGger[:SEQuence]:SOURce <char>



# SCPI Command Tree

---

See a [List of ALL SCPI commands](#)

## **IEEE- 488.2 Common Commands**

### **Local Lockout**

New [See Calibrating the PNA Using SCPI](#)

---

|                    |                                                          |
|--------------------|----------------------------------------------------------|
| <b>ABORt</b>       | Stops all sweeps                                         |
| <b>+ CALCulate</b> | Click to hide and show CALC commands                     |
| <b>:CORRection</b> | Electrical Delay and Phase Offset                        |
| <b>:CUSTom</b>     | Custom measurements                                      |
| <b>:DATA</b>       | Sends and queries data.                                  |
| <b>:FILTer</b>     | Time domain gating                                       |
| <b>:FORMat</b>     | Display format                                           |
| <b>:FSIMulator</b> | Balanced measurements and Fixturing                      |
| <b>:FUNction</b>   | Trace Statistics                                         |
| <b>:LIMit</b>      | Limit lines for pass / fail testing                      |
| <b>:MARKer</b>     | Marker settings                                          |
| <b>:MATH</b>       | Math / Memory                                            |
| <b>:MIXer</b>      | X-axis display for FCA measurments                       |
| <b>:NORMalize</b>  | Receiver power cal (Obsolete)                            |
| <b>:OFFSet</b>     | Mag and Phase offset                                     |
| <b>:PARAmeter</b>  | Create and delete measurements                           |
| <b>:RDATa?</b>     | Queries receiver data                                    |
| <b>:SMOothing</b>  | Point-to-point smoothing                                 |
| <b>:TRANSform</b>  | Time domain transform                                    |
| <b>CONTRol</b>     | Interface control and Rear-panel connector control.      |
| <b>DISPlay</b>     | Display settings                                         |
| <b>FORMat</b>      | Format for data transfer                                 |
| <b>HCOPY</b>       | Hardcopy printing                                        |
| <b>INITiate</b>    | Continuous or manual triggering                          |
| <b>MMEMory</b>     | Saves and recalls instrument states                      |
| <b>OUTPut</b>      | Turns RF power ON and OFF                                |
| <b>ROUTE</b>       | Controls internal switch to reference receiver. (Opt 81) |
| <b>+ SENSE</b>     | Click to hide and show SENSE commands                    |

|                      |                                                    |
|----------------------|----------------------------------------------------|
| <b>:AVERage</b>      | Sweep Averaging                                    |
| <b>:BANDwidth</b>    | IF Bandwidth                                       |
| <b>:CORRection</b>   | Unguided calibration and other correction settings |
| > <b>:CKIT</b>       | Cal Kits                                           |
| > <b>:COLL:CKIT</b>  | Cal Standards                                      |
| > <b>:COLL:GUID</b>  | Guided calibration                                 |
| > <b>:COLL:SESS</b>  | VMC and SMC cals (opt 83)                          |
| > <b>:CSET</b>       | Cal Sets                                           |
| > <b>:EXTensions</b> | Port Extensions                                    |
| <b>:COUPlE</b>       | Chopped or Alternate sweep                         |
| <b>:FREQuency</b>    | Frequency sweep settings                           |
| <b>:IF</b>           | IF Access settings                                 |
| <b>:MIXer</b>        | FCA measurements (opt 83)                          |
| <b>:MULTiplexer</b>  | Controls the E5091A Test Set.                      |
| <b>:OFFSet</b>       | Frequency offset (opt 80)                          |
| <b>:POWer</b>        | Receiver attenuation and overpower protection      |
| <b>:ROSCillator</b>  | Returns the source of the reference oscillator.    |
| <b>:SEGMent</b>      | Segment sweep settings.                            |
| <b>:SWEep</b>        | Sweep types                                        |
| <b>:X:VALues</b>     | Returns X-axis values                              |
| <b>SOURce</b>        | Source power to the DUT                            |
| <b>SOURce:POWer</b>  | Source Power Cal                                   |
| <b>STATus</b>        | Reads the PNA status registers                     |
| <b>SYSTem</b>        | Misc PNA capabilities                              |
| <b>TRIGger</b>       | Trigger measurements                               |

## IEEE 488.2 Common Commands

---

\*CLS - Clear Status

\*ESE - Event Status Enable

\*ESE? - Event Status Enable Query

\*ESR? - Event Status Enable Register

\*IDN? - Identify

\*OPC - Operation complete command

\*OPC? - Operation complete query

\*OPT? - Identify Options Query

\*RST - Reset

\*SRE - Service Request Enable

\*SRE? - Service Request Enable Query

\*STB? - Status Byte Query

\*TST? - Result of Self-test Query

\*WAI - Wait

---

### **\*CLS - Clear Status**

Clears the instrument status byte by emptying the error queue and clearing all event registers. Also cancels any preceding \*OPC command or query. See [Status Commands](#) and [Reading the Analyzer's Status Registers](#).

---

### **\*ESE - Event Status Enable**

Sets bits in the standard event status enable register. See [Status Commands](#) and [Reading the Analyzer's Status Registers](#).

---

### **\*ESE? - Event Status Enable Query**

Returns the results of the standard event enable register. The register is cleared after reading it. See [Status Commands](#) and [Reading the Analyzer's Status Registers](#).

---



### **\*ESR - Event Status Enable Register**

Reads and clears event status enable register. See [Status Commands](#) and [Reading the Analyzer's Status Registers](#).

---

### **\*IDN? - Identify**

Returns a string that uniquely identifies the analyzer. The string is of the form "Agilent Technologies",<model number>,<serial "number">,<software revision>" .

---

### **\*OPC - Operation complete command**

Generates the OPC message in the standard event status register when all pending overlapped operations have been completed (for example, a sweep, or a Default). See [Understanding Command Synchronization](#).

---

### **\*OPC? - Operation complete query**

Returns an ASCII "+1" when all pending overlapped operations have been completed. See [Understanding Command Synchronization](#)

---

#### **\*OPT? - Identify Options Query**

Returns a string identifying the analyzer option configuration.

---

#### **\*RST - Reset**

Executes a device reset and cancels any pending \*OPC command or query, exactly the same as a [SYSTem:PRESet](#). The contents of the analyzer's non-volatile memory are not affected by this command.

---

#### **\*SRE - Service Request Enable**

Before reading a status register, bits must be enabled. This command enables bits in the service request register. The current setting is saved in non-volatile memory. See [Status Commands](#) and [Reading the Analyzer's Status Registers](#).

---

#### **\*SRE? - Service Request Enable Query**

Reads the current state of the service request enable register. The register is cleared after reading it. The return value can be decoded using the table in [Status Commands](#). See also [Reading the Analyzer's Status Registers](#).

---

#### **\*STB? - Status Byte Query**

Reads the value of the instrument status byte. The register is cleared only when the registers feeding it are cleared. See [Status Commands](#) and [Reading the Analyzer's Status Registers](#).

---

#### **\*TST? - Result of Self-test Query**

Returns the result of a query of the analyzer hardware status. An **0** indicates no failures found. Any other value indicates one or more of the following conditions exist. The value returned is the Weight (or sum of the Weights) of the existing conditions. For example:

- If **4** is returned from \*TST?, an **Overpower** condition exists.
- If **6** is returned, both **Unleveled** and **Overpower** conditions exist.

---

| Bit | Weight | Description     | Bit is set to 1 when the following conditions exist:                                                                                                                 |
|-----|--------|-----------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 0   | 1      | Phase Unlock    | The source has lost phaselock. This could be caused by a reference channel open or a hardware failure.                                                               |
| 1   | 2      | Unleveled       | The source power is unleveled. This could be a source is set for more power than it can deliver at the tuned frequency. Or it could be caused by a hardware failure. |
| 2   | 4      | Not used        |                                                                                                                                                                      |
| 3   | 8      | EE Write Failed | An attempted write to the EEPROM has failed. This is possibly caused by a hardware failure.                                                                          |
| 4   | 16     | YIG Cal Failed  | The analyzer was unable to calibrate the YIG. Either the phaselock has been lost or there has been a hardware failure.                                               |

|   |    |                 |                                                                                                    |
|---|----|-----------------|----------------------------------------------------------------------------------------------------|
| 5 | 32 | Ramp Cal Failed | The analyzer was unable to calibrate the analog ramp generator due to a possible hardware failure. |
| 6 | 64 | Not used        |                                                                                                    |

**\*WAI - Wait**

Prohibits the instrument from executing any new commands until all pending overlapped commands have been completed. See [Understanding Command Synchronization](#)

## Abort Command

---

### ABORt

(Write-only) Stops all sweeps - then resume per current trigger settings. This command is the same as INITiate:IMMEDIATE (restart) except if a channel is performing a single sweep, ABORt will stop the sweep, but not initiate another sweep.

|                 |               |
|-----------------|---------------|
| <b>Examples</b> | ABOR<br>abort |
|-----------------|---------------|

|                     |                |
|---------------------|----------------|
| <b>Query Syntax</b> | Not applicable |
|---------------------|----------------|

|                    |    |
|--------------------|----|
| <b>Overlapped?</b> | No |
|--------------------|----|


|                |                |
|----------------|----------------|
| <b>Default</b> | Not applicable |
|----------------|----------------|

---

## Calculate:Correction Commands

---

Controls error correction functions.

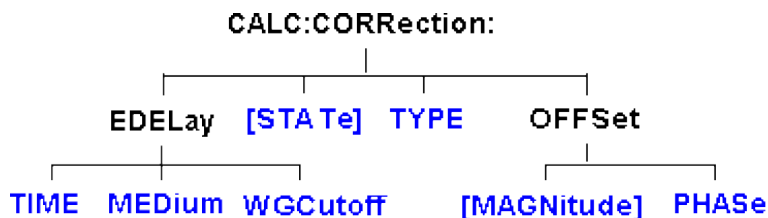

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- New [See Calibrating the PNA Using SCPI](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. To select the measurement use `CALC<ChanNum>:PAR:SEL <MeasName>`.

---

### CALCulate<cnum>:CORRection:EDELay:MEDium <char>

(Read-Write) Sets the media used when calculating the electrical delay.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1.

<num> Choose from: **COAX** for coaxial medium, **WAVE**guide for waveguide medium.

#### Examples

```
CALC:CORR:EDEL:MED COAX
calc3:corr:edelay:medium waveguide
```

**Query Syntax** CALCulate<cnum>:CORRection:EDELay:MEDium?

**Return Type** Character

**Overlapped?** No

**Default** COAX

---

### CALCulate<cnum>:CORRection:EDELay:TIME <num>

(Read-Write) Sets the electrical delay for the selected measurement. **Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Electrical delay in seconds. Choose any number between: **-10.00** and **10.00**  
Use SENS:CORR:RVEL:COAX <num> to set Velocity factor.

**Examples**

```
CALC1:CORR:EDEL:TIME 1NS
calculate2:correction:time 0.5e-12
```

**Query Syntax** CALCulate:CORRection:EDELay:TIME?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 seconds

---

**CALCulate<cnum>:CORRection:EDELay:WGCutoff <num>**

(Read-Write) Sets the waveguide cutoff frequency used when the electrical delay media is set to WAVEguide.  
(See CALCulate:CORRection:EDELay:MEDium <char>.)

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1.

<num> Waveguide cutoff frequency used with the electrical delay calculation.

**Examples**

```
CALC:CORR:EDEL:WGC 18.067 GHz
calculate3:correction:edelay:wgcutoff 14.047 ghz
```

**Query Syntax** CALCulate<cnum>:CORRection:EDELay:WGCutoff?

**Return Type** Numeric

**Overlapped?** No

**Default** 45 MHz

---

**CALCulate<cnum>: CORRection:[STATe] <bool>**



(Read-Write) Turns error correction ON or OFF for the selected measurement on the specified channel.

To turn error correction ON or OFF for a channel, use SENS:CORR:STATE. **Critical Note:**

---

**Note:** You must set the error correction type (CALC:CORR:TYPE) before turning error correction ON.

---

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<bool> Correction state. Choose from:

0 - Correction OFF

1 - Correction ON

**Examples**

```
CALC:CORR ON
```

```
calculate:correction:state off
```

**Query Syntax** CALCulate<cnum>:CORRection:STATe?

**Return Type** Boolean

**Overlapped?** No

**Default** Not Applicable

---

**CALCulate<cnum>:CORRection:TYPE <string>**

(Read-Write) Sets the Cal Type for the selected measurement on the specified channel. This is used when a Cal Set is applied.

---

**Note:** Recent firmware changes have made it such that you should NOT have to set the Cal Type. When you select a Cal Set or perform a calibration, the measurements on the selected channel attempt to find the best calibration type in the Cal Set and turn it on. In addition, changing a measurement parameter (for example, from S11 to S21) will also initiate an attempt to turn calibration on.

---

- Use SENS:CORR:TYPE:CAT? to list the Cal Types in the PNA.
- Use SENS:CORR:CSET:TYPE:CAT? to list the Cal Types contained in the active Cal Set for the channel.
- Use SENS:CORR:COLL:METH to set the Cal type to perform a new calibration,

**Critical Note:**

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<string> Cal Type. Choose from:

- "Full 1 Port"
- "Full 2 Port SOLT"
- "Full 2 Port TRL"
- "Full 3 Port SOLT"
- "Full 4 Port(1,2,3,4)"
- "Open Response"
- "SMC\_2P" or "SMC"
- "SMCRsp+IN"
- "SMCRsp+OUT"
- "SMCRsp"
- "Short Response"
- "Thru Response"
- "Thru Response and Isolation"
- "VMC"

[Learn more applying SMC cal sets](#)

**Examples** `CALC:CORR:TYPE "VMC"`

**Query Syntax** `CALCulate<cnum>:CORRection:TYPE?`

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**CALCulate<cnum>:CORRection:OFFSet[:MAGNitude] <num> OBSOLETE**

(Read-Write) This command is replaced with `SENS:CORR:RPOWer:OFFSet[:AMPLitude]`.  
See an example of a [Receiver Power Calibration](#).

**For Receiver Power Calibration**, specifies the power level to which the selected (unratioed) measurement data is to be adjusted. This command applies only when the selected measurement is of unratioed power. **Critical Note**

To set data trace magnitude offset, use `CALC:OFFS:MAGN`

**Parameters**

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <num> Cal power level in dBm. No limits are enforced on this value, but the PNA receivers themselves have maximum and minimum power specifications (that may differ between PNA models) which this value must comply with for a valid receiver power cal.

**Examples**

```
CALC:CORR:OFFS 10DBM
calculatel:correction:offset:magnitude maximum
```

**Query Syntax** `CALCulate<num>:CORRection:OFFSet[:MAGNitude]?`

**Return Type** Numeric

**Overlapped?** No

**Default** 0dBm

---

**CALCulate<num>:CORRection:OFFSet:PHASe <num>[<char>] OBSOLETE**

This command is replaced with `CALC:OFFS:PHASe`

(Read-Write) Sets the phase offset for the selected measurement. Critical Note:

**Parameters**

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <num> Offset phase value. Choose any number between: **-360** and **360**
- <char> Units for phase. OPTIONAL. Choose either:  
**DEG** - Degrees (default)  
**RAD** - Radians

**Examples**

```
CALC:CORR:OFFS:PHAS 10
calculate:correction:offset:phase 20rad
```

**Query Syntax** `CALCulate:CORRection:OFFSet:PHASe?`

**Return Type** Numeric, returned value always in degrees

**Overlapped?** No


**Default** 0 degrees

---

## Calculate:Custom Commands

---

Provides capability to create and modify Frequency Converter Application (opt 083) measurements.

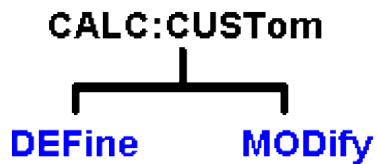

---

### **CALCulate<cnum>:CUSTom:DEFine <Mname>, <ProgID> [,param]**

(Write-only) Creates a custom measurement. The custom measurement is not automatically displayed. You must also do the following:

- Use DISP:WIND:STATe to create a window if it doesn't already exist.
- Use DISP:WIND:TRAC:FEED to display the measurement
- Select the measurement (CALC:PAR:SEL) before making additional settings.

See an example using this command to create a VMC and SMC measurement

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1.

<Mname> Name of the measurement. Any non-empty, unique string, enclosed in quotes.

<ProgID> The type of custom measurement. Choose from:

- FCA.VMCMeas
- SMC\_Forward.SMC\_ForwardMeas
- SMC\_Reverse.SMC\_ReverseMeas



[param] Optional parameter specifies the measurement parameter to create.

| Program ID                  | Valid Parameters:                            |
|-----------------------------|----------------------------------------------|
| FCA.VMCMeas                 | "S11"<br>"VC21"<br>"S22"                     |
| SMC_Forward.SMC_ForwardMeas | "S11"<br>"SC21"<br>"S22"<br>"IPwr"<br>"OPwr" |
| SMC_Reverse.SMC_ReverseMeas | "S11"<br>"SC12"<br>"S22"<br>"IPwr"<br>"OPwr" |

**Examples**

```
CALC2:CUST:DEF 'My VC21', 'FCA.VMCMeas', 'S22'
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

**CALCulate<cnum>:CUSTom:MODify <param>**

(Write-only) Changes the selected custom measurement to a different parameter.

See an example using this command for a VMC and SMC measurement

**Parameters**

<cnum> Channel of the custom measurement to be changed. First, select the measurement using CALC:PAR:SEL.

<param> Parameter to change the custom measurement to. Select a parameter that is valid for the type of measurement.

| Type                    | Valid Parameters                             |
|-------------------------|----------------------------------------------|
| VMC Measurement         | "S11"<br>"VC21"<br>"S22"                     |
| SMC Forward Measurement | "S11"<br>"SC21"<br>"S22"<br>"IPwr"<br>"OPwr" |
| SMC Reverse Measurement | "S11"<br>"SC12"<br>"S22"<br>"IPwr"<br>"OPwr" |

**Examples**

```

SYST:PRES
CALC2:CUST:DEF 'My VC21', 'FCA.VMCMeas'
CALC:PAR:SEL 'My VC21'
CALC2:CUST:MOD 'S22'

```

**Query Syntax** Not applicable


**Overlapped?** No

**Default** Not applicable

## Calculate:Data Commands

---

Controls sending and receiving data with the PNA



- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- See [Data Access Map](#)

---

### **CALCulate<cnum>:DATA <char>,<data>**

Write Writes Measurement data, Memory data, or Normalization Divisor data.

Data type depends on [FORM:DATA](#) command.

**Note:** Calc:Data SCORR command to read / write error terms is OBSOLETE with PNA release 5.0. To write Error Terms, use [SENS:CORR:CSET:DATA](#)

---


### **CALCulate<cnum>:DATA? <char>**

Read Returns Measurement data, Memory data, or Normalization Divisor data.

Data type depends on [FORM:DATA](#) command.

To read Error Terms, use [SENS:CORR:CSET:DATA](#)

To write or read

- **Measurement (DATA)**
- **Memory (MEM)**
-  **Normalization Divisor (DIV)** (Receiver Power Cal error term)



## Parameters

|                     |                                                                                                                                                                                                     |
|---------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>&lt;cnm&gt;</b>  | Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnm> is set to 1.                                                                         |
| <b>&lt;char&gt;</b> | <b>FDATA</b> Formatted trace data from <b>measResult</b> location<br>Returns TWO numbers per data point for Polar and Smith Chart format<br>Returns one number per data point for all other formats |
|                     | <b>SDATA</b> Corrected complex trace data from <b>rawMeas</b> location<br>Returns TWO numbers per data point                                                                                        |
|                     | <b>FMEM</b> Formatted memory data from <b>memResult</b> location<br>Returns TWO numbers per data point for Polar and Smith Chart format<br>Returns one number per data point for all other formats  |
|                     | <b>SMEM</b> Corrected complex data from <b>rawMemory</b> location<br>Returns TWO numbers per data point                                                                                             |
|                     | <b>SDIV</b> Complex data from <b>Normalization Divisor</b> location<br>Returns TWO numbers per data point.                                                                                          |

Notes:

When reading data from, or writing data to, the normalization divisor, you must first create a divisor trace.

If normalization interpolation is ON and the number of points changes after the initial normalization, the divisor data will then be interpolated.

## EXAMPLE

```
CALC:DATA FDATA,Data(x)
calculate2:data sdata,data(r,i)
```

See another [example](#) using this command.

**Return Type:** Block data

**Overlapped?** - No

**Default** - Not Applicable

## Notes:

- When querying memory, you must first store a trace into memory using [CALC:MATH:MEMorize](#).
- When querying the normalization divisor, you must first store a divisor trace using [CALC:NORMalize\[:IMMediate\]](#).
- If normalization interpolation is ON and the number of points changes after the initial normalization, the divisor data will then be interpolated.
- If interpolation is ON and the number of points changes after the initial calibration, the error terms will then be

the interpolated results.

- To get and put receiver data, see [CALC:RDATA?](#)
- To get uncorrected ratioed data, turn correction OFF and use Calc:Data SDATA.
- CALCulate commands act on the selected measurement. You can select one measurement in each channel. Therefore, you can have up to four measurements selected at the same time. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

## **CALCulate<cnum>:DATA:CUSTom <name>,<data>**

(Read-Write) Reads or writes data from a custom-named measurement buffer. Specify the measurement using [CALCulate:PARAmeter:SElect](#). Critical Note:

### **Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <name> Name of the buffer to be read or written
- <data> Data to be read or written to the custom buffer. Format as one number per data point.

**Examples**

```
CALC:DATA:CUST 'VectorResult0',0,1,2,3,4,5 'Write
CALC:DATA:CUST? 'VectorResult0' 'Read
```

**Query Syntax** CALCulate:DATA:CUSTom? <name>

**Return Type** Depends on [Form:Data](#)

**Overlapped?** No

**Default** Not Applicable

---

## **CALCulate<cnum>:DATA:CUSTom:CATalog?**

(Read-only) Reads the list of buffer names (comma separated list of string values) available from the selected parameter. Specify the measurement using CALCulate:PARAmeter:SElect. Critical Note:

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

**Examples**

```
CALC:DATA:CUST:CAT?
calculate:data:custom:catalog?
```

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**CALCulate<cnum>:DATA:SNP? <n>**

(Read-only) Reads SnP data from the selected measurement. Learn more about SnP data. Critical Note:

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<n> Amount of data to return. If unspecified, <n> is set to 2. Choose from:

**1** (S1P) returns data for the active measurement.

**2** (S2P) returns data for the 2 port parameters associated with the current measurement. Default.

**3** (S3P) returns data for the 3 port parameters associated with the current measurement. Valid only on instruments with more than 2 ports.

SnP data can be output using several data formatting options. See the command MMEM:STORe:TRACe:FORMat:SNP.

See also MMEM:STOR <file>.<snp>

**Examples**

```
CALC:PAR:DEF "MyMeasurement", S11
CALC:PAR:SEL "MyMeasurement"
CALC:DATA:SNP? 1
```

**Return Type** Depends on FORMat:DATA

**Overlapped?** No

**Default** Not Applicable


---



## Calculate:Filter Commands

---

Controls the gating function used in time domain measurements. The gated range is specified with either (start / stop) or (center / span) commands.

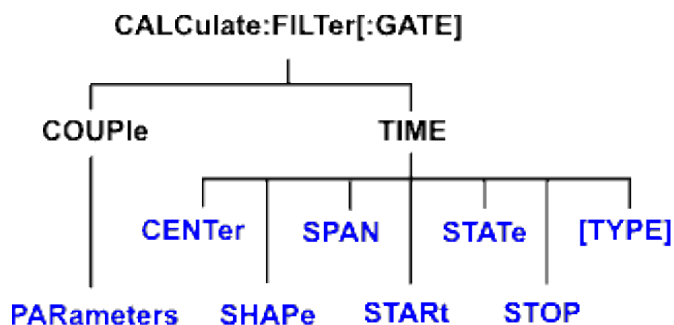

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Gating](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

### **CALCulate<cnum>:FILTer[:GATE]:COUPlE:PARAmeters <num>**

(Read-Write) Specifies the time domain gating parameters to be coupled. The settings for those parameters will be copied from the selected measurement to all other measurements on the channel.

- To enable Trace Coupling, use [SENS:COUP:PAR](#)
- To specify Transform parameters to couple, use [CALC:TRAN:COUP:PAR](#)

 [Learn more about Time Domain Trace Coupling](#)

#### **Critical Note:**

##### **Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <num> (Numeric) Parameters to couple. To specify more than one parameter, add the numbers.
- 1 - Gating Stimulus (Start, Stop, Center, and Span TIME settings.)
  - 2 - Gating State (ON / OFF)
  - 4 - Gating Shape (Minimum, Normal, Wide, and Maximum)
  - 8 - Gating Type (Bandpass and Notch)

**Examples** 'To couple all parameters:  
CALC:FILT:COUP:PAR 15  
'To couple Stimulus and Type:  
calculate2:filter:gate:couple:parameters 9

**Query Syntax** CALCulate<cnum>:FILTer:GATE:COUPle:PARameters?

**Return Type** Numeric

**Overlapped?** No

**Default** 13 (All parameters except 2 - Gating State)

---

### CALCulate<cnum>:FILTer[:GATE]:TIME:CENTer <num>

(Read-Write) Sets the gate filter center time. **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Center time in seconds; Choose any number between:  
 $\pm (\text{number of points}-1) / \text{frequency span}$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples** CALC:FILT:GATE:TIME:CENT -5 ns  
calculate2:filter:time:center maximum

**Query Syntax** CALCulate<cnum>:FILTer[:GATE]:TIME:CENTer?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### CALCulate<cnum>:FILTer[:GATE]:TIME:SHAPe <char>

(Read-Write) Sets the gating filter shape when in time domain. **Critical Note:**

**Parameters**

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <char> Choose from  
**MAXimum** - the widest gate filter available  
**WIDE** -  
**NORMAL** -  
**MINimum** - the narrowest gate filter available

**Examples**

```
CALC:FILT:GATE:TIME:SHAP MAX
calculate2:filter:time:shape normal
```

**Query Syntax** CALCulate<num>:FILTer[:GATE]:TIME:SHAPE?

**Return Type** Character

**Overlapped?** No

**Default** NORMAl

---

**CALCulate<num>:FILTer[:GATE]:TIME:SPAN <num>**

(Read-Write) Sets the gate filter span time. **Critical Note:**

**Parameters**

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <num> Time span in seconds; Choose any number between:  
**0** and  $2 * [(number\ of\ points - 1) / frequency\ span]$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
CALC:FILT:GATE:TIME:SPAN 5 ns
calculate2:filter:time:span maximum
```

**Query Syntax** CALCulate<num>:FILTer[:GATE]:TIME:SPAN?

**Return Type** Numeric

**Overlapped?** No

**Default** 20 ns

---

**CALCulate<num>:FILTer[:GATE]:TIME:STATe <boolean>**

(Read-Write) Turns gating state ON or OFF. **Critical Note:**

**Note:** Sweep type must be set to LLinear Frequency in order to use Transform Gating.

---

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<boolean> **ON** (or 1) - turns gating ON.  
**OFF** (or 0) - turns gating OFF.

**Examples**

```
CALC:FILT:TIME:STAT ON
calculate2:filter:gate:time:state off
```

**Query Syntax** CALCulate<cnum>:FILTer[:GATE]:TIME:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**CALCulate<cnum>:FILTer[:GATE]:TIME:STARt <num>**

(Read-Write) Sets the gate filter start time. **Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Start time in seconds; any number between:  
 $\pm (\text{number of points}-1) / \text{frequency span}$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
CALC:FILT:TIME:STAR 1e-8
calculate2:filter:gate:time:start minimum
```

**Query Syntax** CALCulate<cnum>:FILTer[:GATE]:TIME:STARt?

**Return Type** Numeric

**Overlapped?** No

**Default** 10 ns

---

**CALCulate<cnum>:FILTer[:GATE]:TIME:STOP <num>**



(Read-Write) Sets the gate filter stop time. **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<num> Stop time in seconds; any number between:  
 $\pm (\text{number of points}-1) / \text{frequency span}$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
CALC:FILT:TIME:STOP -1 ns
calculate2:filter:gate:time:stop maximum
```

**Query Syntax** CALCulate<num>:FILTer[:GATE]:TIME:STOP?

**Return Type** Numeric

**Overlapped?** No

**Default** 10 ns

---

**CALCulate<num>:FILTer[:GATE]:TIME[:TYPE] <char>**

(Read-Write) Sets the type of gate filter used. **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<char> Choose from:  
**BPASs** - Includes (passes) the range between the start and stop times.  
**NOTCh** - Excludes (attenuates) the range between the start and stop times.

**Examples**

```
CALC:FILT:TIME BPAS
calculate2:filter:gate:time:type notch
```

**Query Syntax** CALCulate<num>:FILTer[:GATE]:TIME[:TYPE]?

**Return Type** Character

**Overlapped?** No

**Default** BPAS

---

## Calculate:Format Command

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using `CALC:PAR:SEL`.

---

- See an [example](#) using this command.
  - See a [List](#) of all commands in this block.
  - [Learn About Data Format](#)
- 

### CALCulate<cnum>:FORMat <char>

(Read-Write) Sets the display format for the measurement. **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<char> Choose from:

- MLINear
- MLOGarithmic
- PHASe
- IMAGinary
- REAL
- POLar
- SMITH
- SWR
- GDElay



#### Examples

```
CALC:FORM MLIN
calculate2:format polar
```

**Query Syntax** CALCulate<cnum>:FORMat?

**Return Type** Character

**Overlapped?** No


**Default** MLINear

---

## Calculate:FSimulator Commands

---

Specifies settings and fixturing for Balanced Measurements.

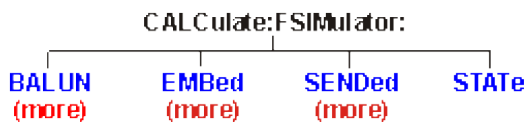

- Click a **blue** keyword to view the command details.
  - See a [List](#) of all SCPI commands.
- 

### CALCulate<num>:FSIMulator:STATe <bool>

(Read-Write) Turns all three fixturing functions (de-embedding, port matching, impedance conversion) ON or OFF for all ports on the specified channel. Does not affect port extensions.

**Note:** This command affects ALL measurements on the specified channel.

---

#### Parameters

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <bool> Choose from:  
**ON or 1** - Turns Fixturing ON  
**OFF or 0** - Turns Fixturing OFF

#### Examples

```
CALC:FSIM:STAT 1
calculate2:fsimulator:state 0
```

**Query Syntax** CALCulate<num>:FSIMulator:STATe?

**Return Type** Boolean


**Overlapped?** No

**Default** OFF

---

## Calculate:Function Commands

---

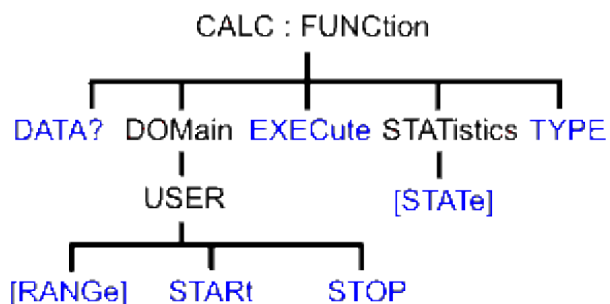

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Trace Statistics](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

### CALCulate<cnum>:FUNCtion:DATA?

(Read-only) Returns the trace statistic data for the selected statistic type for the specified channel. Select the type of statistic with [CALC:FUNC:TYPE](#). **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

**Return Type** Depends on [FORM:DATA](#)

**Example** `CALCulate2:FUNCtion:DATA?`

**Overlapped?** No

**Default** Not applicable

---

### CALCulate<cnum>:FUNCtion:DOMain:USER[:RANGe] <range>

(Read-Write) Sets the range used to calculate trace statistics. Each channel has 16 user ranges. The x-axis range is specified with the CALC:FUNC:DOM:USER:START and STOP commands. **Critical Note:**

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <range> Range number. Choose from: **0 to 16**  
**0** is Full Span of the current x-axis range  
**1 to 16** are user-specified ranges

**Examples**

```
CALC:FUNC:DOM:USER 4
calculate2:function:domain:user:range 0
```

**Query Syntax** CALCulate<cnun>:FUNction:DOMain:USER[:RANGe]?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 - Full Span

---

**CALCulate<cnun>:FUNction:DOMain:USER:STARt <range>, <start>**

(Read-Write) Sets the start of the specified user-domain range.

To apply this range, use CALC:FUNC:DOM:USER

To set the stop of the range, use CALC:FUNC:DOM:USER:STOP. **Critical Note:**

**Note:** This command does the same as CALC:MARK:FUNC:DOM:USER:STAR

---

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <range> Range number that will receive the start value. Choose an integer between **1** and **16**
- <start> Start value of the specified range. Choose a real number between: the analyzer's **Minimum** and **Maximum** x-axis value.

**Examples**

```
CALC:FUNC:DOM:USER:STAR 1,1e9
calculate2:function:domain:user:start 2,2e9
```

**Query Syntax** CALCulate<cnun>:FUNction:DOMain:USER:STARt? <range>

**Return Type** Numeric

**Overlapped?** No

**Default** The analyzer's **Minimum** x-axis value

---

## CALCulate<cnum>:FUNction:DOMain:USER:STOP <range>, <stop>

(Read-Write) Sets the stop value of the specified user-domain range.

To apply this range, use CALC:FUNC:DOM:USER.

To set the start of the range, use CALC:FUNC:DOM:USER:START

Critical Note:

---

**Note:** This command does the same as CALC:MARK:FUNC:DOM:USER:STOP

---

### Parameters

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <range> Range number that will receive the stop value. Choose an integer between **1** and **16**
- <stop> Stop value of the specified range. Choose a real number between: the analyzer's **Minimum** and **Maximum** x-axis value.

### Examples

```
CALC:FUNC:DOM:USER:STOP 4,5e9
calculate2:function:domain:user:stop 3,8e9
```

**Query Syntax** CALCulate<cnum>:FUNction:DOMain:USER:STOP? <range>

**Return Type** Numeric

**Overlapped?** No

**Default** The analyzer's **Maximum** x-axis value

---

## CALCulate<cnum>:FUNction:EXECute

(Write-only) For the active trace of specified channel, executes the statistical analysis specified by the CALC:FUNC:TYPE command. **Critical Note:**

### Parameters

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

### Examples

```
CALC:FUNC:EXEC
calculate2:function:execute
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## CALCulate<cnum>:FUNction:STATistics[:STATe] <ON|OFF>

(Read-Write) Displays and hides the trace statistics (peak-to-peak, mean, standard deviation) on the screen. The analyzer will display either measurement statistics or Filter Bandwidth statistics; not both. **Critical Note:**

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <ON|OFF> ON - Displays trace statistics  
OFF - Hides trace statistics

**Examples**

```
CALC:FUNC:STAT ON
calculate2:function:statistics:state off
```

**Query Syntax** CALCulate<cnun>:FUNCtion:STATistics[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF (0)

**CALCulate<cnun>:FUNCtion:TYPE <char>**

(Read-Write) Sets statistic TYPE that you can then query using CALC:FUNCtion:DATA?.

**Note:** In PNA releases 4.2 and prior, this command applied the statistic type to all measurements. Now, this command affects only the selected measurement on the specified channel.

Critical Note:

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <char> Choose from:
  - PTPeak** - the difference between the max and min data points on the trace.
  - STDEV** - standard deviation of all data points on the trace
  - MEAN** - mean (average) of all data points on the trace
  - MIN** - lowest data point on the trace
  - MAX** - highest data point on the trace

**Examples**

```
CALC:FUNC:TYPE PTP
calculate2:function:type stdev
```

**Query Syntax** CALCulate<cnun>:FUNCtion:TYPE?

**Return Type** Character

**Overlapped?** No


Default PTPeak

---



## Calc:Limit Commands

Controls the limit segments used for pass / fail testing.

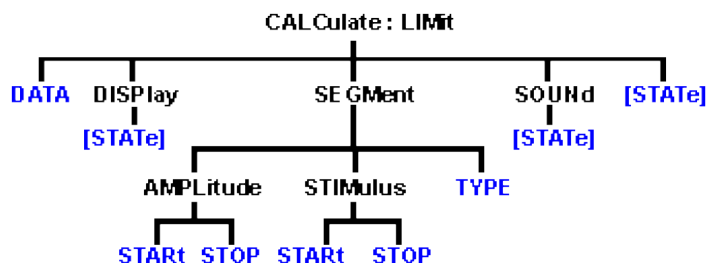

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Limit Lines](#)

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

### CALCulate<cnum>:LIMit:DATA <block>

(Read-Write) Sets data for limit segments. **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<block> Data for all limit segments in REAL,64 format. The following is the data format for 1 segment:

**Type,BegStim, EndStim, BegResp,EndResp**



**Type** Type of limit segment. Choose from  
 0 - Off  
 1 - Max  
 2 - Min

**BegStim** Start of X-axis value (freq, power, time)

**EndStim** End of X-axis value

**BegResp** Y-axis value that corresponds with Start of X-axis value

**EndResp** Y-axis value that corresponds with End of X-axis value

#### Examples

The following writes three max limit segments for a bandpass filter.

```
"CALC:LIM:DATA 1,3e5,4e9,-60,0,1,4e9,7.5e9,0,0,1,7.5e9,9e9,0,-30"
```

**Query Syntax** CALCulate<cnum>:LIMit:DATA?

**Return Type** Depends on FORM:DATA - All 100 predefined limit segments are returned.

**Overlapped?** No

**Default** 100 limit segments - all values set to 0

---

### **CALCulate<cnum>:LIMit:DISPlay[:STATe] <ON | OFF>**

(Read-Write) Turns the display of limit segments ON or OFF (if the data trace is turned ON). **Critical Note:**

#### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<ON | OFF> **ON** (or 1) - turns the display of limit segments ON.  
**OFF** (or 0) - turns the display of limit segments OFF.

#### **Examples**

```
CALC:LIM:DISP:STAT ON
calculate2:limit:display:state off
```

**Query Syntax** CALCulate<cnum>:LIMit:DISPlay[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

### **CALCulate<cnum>:LIMit:SEGMENT<snum>AMPLitude:STARt <num>**

(Read-Write) Sets the start (beginning) of the Y-axis amplitude (response) value. **Critical Note:**

#### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<snum> Segment number; if unspecified, value is set to 1.

<num> Choose any number between: **-500** and **500**

Display value is limited to the Maximum and Minimum displayed Y-axis values.

#### **Examples**

```
CALC:LIM:SEGM1:AMPL:STAR 10
calculate2:limit:segment2:amplitude:start 10
```

**Query Syntax** CALCulate<cnum>:LIMit:SEGMENT<snum>AMPLitude:STARt?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:LIMit:SEGMENT<snum>AMPLitude:STOP <num>**

(Read-Write) Sets the stop (end) of the Y-axis amplitude (response) value. **Critical Note:**

#### **Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <snum> Segment number; if unspecified, value is set to 1.
- <num> Choose any number between: **-500** and **500**  
Display value is limited to the Maximum and Minimum displayed Y-axis values.

#### **Examples**

```
CALC:LIM:SEGM1:AMPL:STOP 10
calculate2:limit:segment2:amplitude:stop 10
```

**Query Syntax** CALCulate<cnum>:LIMit:SEGMENT<snum>AMPLitude:STOP?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:LIMit:SEGMENT<snum>STIMulus:START <num>**

(Read-Write) Sets the start (beginning) of the X-axis stimulus value. **Critical Note:**

#### **Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <snum> Segment number; if unspecified, value is set to 1.
- <num> Choose any number within the X-axis span of the analyzer.

#### **Examples**

```
CALC:LIM:SEGM1:STIM:STAR 10
calculate2:limit:segment2:stimulus:start 10
```

**Query Syntax** CALCulate<cnum>:LIMit:SEGMENT<snum>STIMulus:START?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## CALCulate<cnum>:LIMit:SEGMENT<snum>STIMulus:STOP <num>

(Read-Write) Sets the stop (end) of the X-axis stimulus value. **Critical Note:**

### Parameters

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <snum> Segment number; if unspecified, value is set to 1.
- <num> Choose any number within the X-axis span of the analyzer.

### Examples

```
CALC:LIM:SEGM1:AMPL:STOP 10
calculate2:limit:segment2:stimulus:stop 10
```

**Query Syntax** CALCulate<cnum>:LIMit:SEGMENT<snum>STIMulus:STOP?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## CALCulate<cnum>:LIMit:SEGMENT<snum>:TYPE <char>

(Read-Write) Sets the type of limit segment. **Critical Note:**

### Parameters

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <snum> Segment number. Choose any number between:  
**1** and **100**  
If unspecified, value is set to 1.
- <char> Choose from:  
**LMAX** - a MAX limit segment. Any response data exceeding the MAX value will fail.  
**LMIN** - a MIN limit segment. Any response data below the MIN value will fail.  
**OFF** - the limit segment (display and testing) is turned OFF.

### Examples

```
CALC:LIM:SEGM:TYPE LMIN
calculate2:limit:segment3:type lmax
```

**Query Syntax** CALCulate<cnum>:LIMit:SEGMENT<snum>:TYPE?

**Return Type** Character

**Overlapped?** No

**Default** OFF

---

## CALCulate<cnum>:LIMit:SOUNd[:STATe] <ON | OFF>

(Read-Write) Turns limit testing fail sound ON or OFF. **Critical Note:**

### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<ON | OFF> **ON** (or 1) - turns sound ON.  
**OFF** (or 0) - turns sound OFF.

### Examples

```
CALC:LIM:SOUN ON
calculate2:limit:sound:state off
```

**Query Syntax** CALCulate<cnum>:LIMit:SOUNd[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

## CALCulate<cnum>:LIMit:STATe <ON | OFF>

(Read-Write) Turns limit segment **testing** ON or OFF.

- Use CALC:LIM:DISP to turn ON and OFF the **display** of limit segments.
- If using Global Pass/Fail status, trigger the PNA AFTER turning Limit testing ON.
- **Critical Note:**

### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<ON | OFF> **ON** (or 1) - turns limit testing ON.  
**OFF** (or 0) - turns limit testing OFF.

### Examples

```
CALC:LIM:STAT ON
calculate2:limit:state off
```

**Query Syntax** CALCulate<cnum>:LIMit:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No


**Default** OFF

---

## Calculate:Marker Commands

---

Controls the marker settings used to remotely output specific data to the computer.

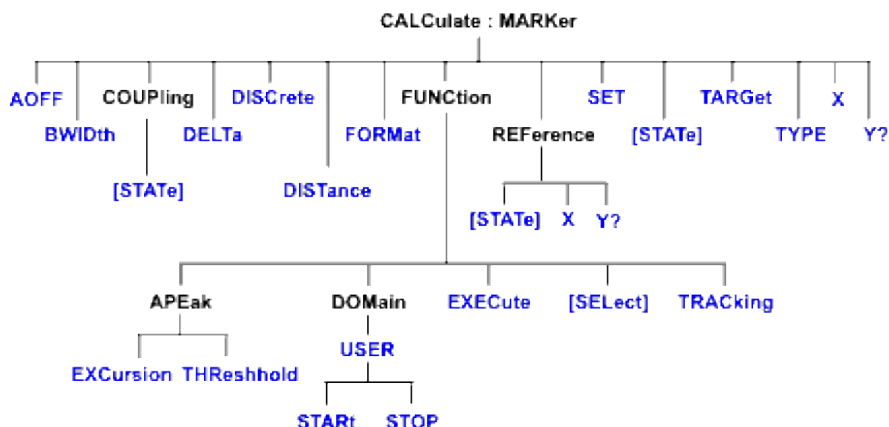

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- See Marker Readout [number](#) and [size](#) commands.
- [Learn about Markers](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

**Note:** The Reference Marker is Marker Number 10

---

### CALCulate<cnum>:MARKer:AOFF

(Write-only) Turns all markers off for selected measurement. **Critical Note:**

#### Parameters



<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

#### Examples

```
CALC:MARK:AOFF
calculate2:marker:aoff
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

### CALCulate<cnum>:MARKer:BWIDth <num>

(Read-Write) Turns on and sets markers 1 through 4 to calculate filter bandwidth. The <num> parameter sets the value below the maximum bandwidth peak that establishes the bandwidth of a filter. For example, if you want to determine the filter bandwidth 3 db below the bandpass peak value, set <num> to -3.

This feature activates markers 1 through 4. To turn off these markers, either turn them off individually or turn them All Off.

The analyzer screen will show either Bandwidth statistics OR Trace statistics; not both.

To search a User Range with the bandwidth search, first activate marker 1 and set the desired User Range. Then send the CALC:MARK:BWID command. The user range used with bandwidth search only applies to marker 1 searching for the max value. The other markers may fall outside the user range.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Target value below filter peak. Choose any number between **-500** and **500**

**Examples**

```
CALC:MARK:BWID -3
calculate2:marker:bwid -2.513
```

**Query Syntax** CALCulate<cnum>:MARKer:BWIDth?  
Returns the results of bandwidth search:

**Return Type** Numeric - Four Character values separated by commas: bandwidth, center Frequency, Q, loss.

**Overlapped?** No

**Default** -3

---

**CALCulate<cnum>:MARKer<mkr>:COUPling[:STATe]<ON|OFF>**

(Read-Write) Sets and Reads the state of Coupled Markers (ON and OFF) **Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any existing marker number from 1 to 10; if unspecified, value is set to 1.

<ON|OFF> **False (0)** - Turns Coupled Markers OFF

**True (1)** - Turns Coupled Markers ON

**Examples**

```
CALC:MARK:COUP ON
calculate2:marker8:coupling off
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:COUPling:[STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

### **CALCulate<cnum>:MARKer<mkr>:DELTA <ON|OFF>**

(Read-Write) Specifies whether marker is relative to the Reference marker or absolute.

**Note:** The reference marker must already be turned ON with CALC:MARK:REF:STATE.

---

#### **Critical Note:**

#### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any existing marker number from 1 to 10; if unspecified, value is set to 1.

<ON|OFF> **ON** (or 1) - Specified marker is a Delta marker  
**OFF** (or 0) - Specified marker is an ABSOLUTE marker

#### **Examples**

```
CALC:MARK:DELTA ON
calculate2:marker8:delta off
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:DELTA?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

### **CALCulate<cnum>:MARKer<mkr>:DIScrete <ON|OFF>**



(Read-Write) Makes the specified marker display either a calculated value between data points (interpolated data) or the actual data points (discrete data). **Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any existing marker number from 1 to 10; if unspecified, value is set to 1.

<ON|OFF> **ON** (or 1) - Specified marker displays the actual data points  
**OFF** (or 0) - Specified marker displays calculated data between the actual data points.

**Examples**

```
CALC:MARK:DISC ON
calculate2:marker8:discrete off
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:DISCrite?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**CALCulate<cnum>:MARKer<mkr>:DISTance <num>**

(Read-Write) Set or query marker distance on a time domain trace.

The Write command moves the marker to the specified distance value. Once moved, you can read the Y axis value or read the X-axis time value. (Distance is calculated from the X-axis time value.)

The Read command reads the distance of the marker.

If the marker is set as delta, the WRITE and READ data is relative to the reference marker.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any existing marker number from 1 to 10; if unspecified, value is set to 1.

<num> Marker distance in the unit of measure specified with CALC:TRAN:TIME:MARK:UNIT

**Examples**

```
CALC:MARK:DIST .1
calculate2:marker8:distance 5
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:DISTance?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

## **CALCulate<cnum>:MARKer<mkr>:FORMat <char>**

(Read-Write) Sets the format of the data that will be returned in a marker data query CALC:MARK:Y? and the displayed value of the marker readout. The selection does not have to be the same as the measurement's display format. **Critical Note:**

### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any marker number from 1 to 10; if unspecified, value is set to 1

<char> Choose from:

**DEFault** - The format of the selected measurement

**MLINear** - Linear magnitude

**MLOGarithmic** - Logarithmic magnitude

**IMPedance** - (R+jX)

**ADMittance** - (G+jB)

**PHASe** - Phase

**IMAGinary** - Imaginary part (Im)

**REAL** - Real part (Re)

**POLar** - (Re, Im)

**GDELay** - Group Delay

**LINPhase** - Linear Magnitude and Phase

**LOGPhase** - Log Magnitude and Phase

### **Examples**

```
CALC:MARK:FORMat MLIN
calculate2:marker8:format Character
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:FORMat?

**Return Type** Character

**Overlapped?** No

**Default** DEFault

---

## **CALCulate<cnum>:MARKer<mkr>:FUNCtion:APEak:EXCursion <num>**

(Read-Write) Sets amplitude peak excursion for the specified marker. The Excursion value determines what is considered a "peak". This command applies to marker peak searches (Next peak, Peak Right, Peak Left).

**Critical Note:**

**Parameters**

- <cnm> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnm> is set to 1.
- <mkr> Any existing marker number from 1 to 10; if unspecified, value is set to 1.
- <num> Excursion value. Choose any number between **-500** and **500**.

---

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
CALC:MARK:FUNC:APE:EXC 10
calculate2:marker8:function:apeak:excursion maximum
```

**Query Syntax** CALCulate<cnm>:MARKer<mkr>:FUNction:APEak:EXCursion?

**Return Type** Numeric

**Overlapped?** No

**Default** 3

---

**CALCulate<cnm>:MARKer<mkr>:FUNction:APEak:THReshold <num>**

(Read-Write) Sets peak threshold for the specified marker. If a peak (using the criteria set with :EXCursion) is below this reference value, it will not be considered when searching for peaks. This command applies to marker peak searches (Next peak, Peak Right, Peak Left). **Critical Note:**

**Parameters**

- <cnm> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnm> is set to 1.
- <mkr> Any marker number from 1 to 10; if unspecified, value is set to 1
- <num> Threshold value. Choose any number between **-500** and **500**.

---

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
CALC:MARK:FUNC:APE:THR -40
calculate2:marker8:function:apeak:threshold -55
```

**Query Syntax** CALCulate<cnm>:MARKer<mkr>:FUNction:APEak:THReshold?

**Return Type** Numeric

**Overlapped?** No

### **CALCulate<cnum>:MARKer<mkr>:FUNcTion:DOMain:USER <range>**

(Read-Write) Assigns the specified marker to a range number. The x-axis travel of the marker is constrained to the range's span. The span is specified with the CALC:MARK:FUNC:DOM:USER:START and STOP commands, unless range 0 is specified which is the full span of the analyzer.

Each channel has **16** user ranges. (Trace statistics use the same ranges.) More than one marker can use a domain range. **Critical Note:**

#### **Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <mkr> Any marker number from 1 to 10; if unspecified, value is set to 1
- <span> User span. Choose any Integer from **0 to 16**  
**0** is Full Span of the analyzer  
**1 to 16** are available for user-defined x-axis span

#### **Examples**

```
CALC:MARK:FUNC:DOM:USER 1
calculate2:marker8:function:domain:user 1
```

#### **Query Syntax**

CALCulate<cnum>:MARKer<mkr>:FUNcTion:DOMain:USER?  
Returns the user span number that the specified marker is assigned to.

#### **Return Type**

Numeric

#### **Overlapped?**

No

#### **Default**

0 - Full Span

---

### **CALCulate<cnum>:MARKer<mkr>:FUNcTion:DOMain:USER:START <start>**

(Read-Write) Sets the start of the span that the specified marker's x-axis span will be constrained to.

Use `CALC:MARK:FUNC:DOM:USER<range>` to set range number

Use `CALC:MARK:FUNC:DOM:USER:STOP` to set the stop value.

---

**Note:** If the marker is assigned to range 0 (full span), the USER:START and STOP commands generate an error. You cannot set the START and STOP values for "Full Span".

---

**Note:** This command does the same as `CALC:FUNC:DOM:USER:STAR`

---

**Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <mkr> Any marker number from 1 to 10; if unspecified, value is set to 1
- <start> The analyzer's **Minimum** x-axis value

**Examples**

```
CALC:MARK:FUNC:DOM:USER:START 500E6
calculate2:marker8:function:domain:user:start 1e12
```

**Query Syntax** `CALCulate<cnum>:MARKer<mkr>:FUNction:DOMain:USER:START?`

**Return Type** Numeric

**Overlapped?** No

**Default** The analyzer's **Minimum** x-axis value

---

**CALCulate<cnum>:MARKer<mkr>:FUNction:DOMain:USER:STOP <stop>**

(Read-Write) Sets the stop of the span that the marker's x-axis travel will be constrained to.

Use `CALC:MARK:FUNC:DOM:USER<range>` to set range number

Use `CALC:MARK:FUNC:DOM:USER:START` to set the stop value.

---

**Note:** If the marker is assigned to range 0 (full span), the USER:START and STOP commands generate an error. You cannot set the START and STOP values for "Full Span".

---

**Note:** This command does the same as `CALC:FUNC:DOM:USER:STOP`

---

**Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.
- <stop> Stop value of x-axis span; Choose any number between the analyzer's **MINimum** and **MAXimum** x-axis value.

**Examples** `CALC:MARK:FUNC:DOM:USER:STOP 500e6`  
`calculate2:marker8:function:domain1:user:stop 1e12`

**Query Syntax** `CALCulate<cnum>:MARKer<mkr>:FUNCTion:DOMain:USER:STOP?`

**Return Type** Numeric

**Overlapped?** No

**Default** The analyzer's **MAXimum** x-axis value.

---

## **CALCulate<cnum>:MARKer<mkr>:FUNCTion:EXECute [<func>]**

(Write-only) Immediately executes (performs) the specified search function. If no function is specified, executes the selected function. Select the function with `CALC:MARK:FUNCTion:SEL`. **Critical Note:**

### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.

<func> Optional argument. The function that is to be performed. Choose from:

- **MAXimum** - finds the highest value
- **MINimum** - finds the lowest value
- **RPEak** - finds the next valid peak to the right
- **LPEak** - finds the next valid peak to the left
- **NPEak** - finds the next highest value among the valid peaks
- **TARGET** - finds the target value to the right, wraps around to the left
- **LTARGET** - finds the next target value to the left of the marker
- **RTARGET** - finds the next target value to the right of the marker

**Examples** `CALC:MARK:FUNC:EXEC`  
`calculate2:marker2:function:execute maximum`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

## **CALCulate<cnum>:MARKer<mkr>:FUNCTion[:SElect] <char>**

(Read-Write) Sets the search function that the specified marker will perform when executed. To execute (or perform) the function, use:

CALC:MARK:FUNC:EXEC or

CALC:MARK:FUNC:TRAC ON to automatically execute the search every sweep. **Critical Note:**

### Parameters

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.

<char> Marker function. Choose from:

- **MAXimum** - finds the highest value
- **MINimum** - finds the lowest value
- **RPEak** - finds the next valid peak to the right
- **LPEak** - finds the next valid peak to the left
- **NPEak** - finds the next highest value among the valid peaks
- **TARGet** - finds the target value to the right, wraps around to the left
- **LTARget** - finds the next target value to the left of the marker
- **RTARget** - finds the next target value to the right of the marker

### Examples

```
CALC:MARK:FUNC MAX
calculate2:marker8:function:select ltarget
```

**Query Syntax** CALCulate<num>:MARKer<mkr>:FUNction[:SElect]?

**Return Type** Character

**Overlapped?** No

**Default** MAX

---

**CALCulate<num>:MARKer<mkr>:TARGet <num>**

(Read-Write) Sets the target value for the specified marker when doing Target Searches with CALC:MARK:FUNC:SEL <TARGet | RTARget | LTARget> **Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.
- <num> Target value to search for; Units are NOT allowed.

**Examples**

```
CALC:MARK:TARG 2.5
calculate2:marker8:target -10.3
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:TARGet?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**CALCulate<cnum>:MARKer<mkr>:FUNCtion:TRACking <ON | OFF>**

(Read-Write) Sets the tracking capability for the specified marker. The tracking function finds the selected search function every sweep. In effect, turning Tracking ON is the same as doing a CALC:MARK:FUNC:EXECute command every sweep. **Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.
- <ON | OFF> **ON** (or 1) - The specified marker will "Track" (find) the selected function every sweep.  
**OFF** (or 0) - The specified marker will find the selected function **only** when the CALC:MARK:FUNC:EXECute command is sent.

**Examples**

```
CALC:MARK:FUNC:TRAC ON
calculate2:marker8:function:tracking off
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:FUNCtion:TRACking?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---



## CALCulate<cnum>:MARKer:REFerence[:STATe] <ON | OFF>

(Read-Write) Turns the reference marker (marker 10) ON or OFF. When turned OFF, existing Delta markers revert to absolute markers. **Critical Note:**

### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<ON | OFF> **ON** (or 1) - turns reference marker ON  
**OFF** (or 0) - turns reference marker ON

### Examples

```
CALC:MARK:REF ON
calculate2:marker:reference:state OFF
```

**Query Syntax** CALCulate<cnum>:MARKer:REFerence[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

## CALCulate<cnum>:MARKer:REFerence:X <num>

(Read-Write) Sets and returns the absolute x-axis value of the reference marker (marker 10). **Critical Note:**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> X-axis value. Choose any number within the operating domain of the reference marker.

### Examples

```
CALC:MARK:REF:X 1e9
calculate2:marker:reference:x 1e6
```

**Query Syntax** CALCulate<cnum>:MARKer:REFerence:X?

**Return Type** Numeric

**Overlapped?** No

**Default** If the first Marker, turns ON in the middle of the X-axis span. If not, turns ON at the position of the active marker.

---

## CALCulate<cnum>:MARKer:REFerence:Y?

(Read-only) Returns the absolute Y-axis value of the reference marker. **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

**Examples**

```
CALC:MARK:REF:Y?
calculate2:marker:reference:y?
```

**Return Type** Character

**Overlapped?** No

**Default** Not applicable

---

**CALCulate<num>:MARKer<mrk>:TYPE <char>**

(Read-Write) Sets the type of the specified marker. **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<mrk> Any marker number from 1 to 10; if unspecified, value is set to 1

<char> Choose from:

- **NORMal** - a marker that stays on the assigned X-axis position unless moved or searching.
- **FIXed** - a marker that will not leave the assigned X or current Y-axis position.

**Examples**

```
CALC:MARK:TYPE NORM
calculate2:marker2:type fixed
```

**Query Syntax** CALCulate<num>:MARKer<mrk>:TYPE?

**Return Type** Character

**Overlapped?** No

**Default** NORMal

---

**CALCulate<num>:MARKer<mrk>:SET <char>**

(Read-Write) Sets the selected instrument setting to assume the value of the specified marker.

Marker Functions CENT, SPAN, START, and STOP do not work with channels that are in CW or Segment Sweep mode.

Critical Note:

### Parameters

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <mr> Any marker number from 1 to 10; if unspecified, value is set to 1
- <chr> Choose from:
- **CENTer** - changes center frequency to the value of the marker
  - **SPAN** - changes the sweep span to the span that is defined by the delta marker and the marker that it references. Unavailable if there is no delta marker.
  - **START** - changes the start frequency to the value of the marker
  - **STOP** - changes the stop frequency to the value of the marker
  - **RLEVel** - changes the reference level to the value of the marker
  - **DELay** - changes the line length at the receiver input to the phase slope at the active marker stimulus position.

### Examples

```
CALC:MARK:SET CENT
calculate2:marker8:set span
```

**Query Syntax** CALCulate<num>:MARKer<mr>:SET?

**Return Type** Character

**Overlapped?** No

**Default** Not applicable

---

**CALCulate<num>:MARKer<mr>[:STATe] <ON|OFF>**

(Read-Write) Turns the specified marker ON or OFF. **Marker 10 is the Reference Marker.** To turn all markers off, use CALC:MARK:AOFF. **Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.

<ON|OFF> **ON** (or 1) - turns marker ON.  
**OFF** (or 0) - turns marker OFF.

**Examples**

```
CALC:MARK ON
calculate2:marker8 on
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** Off

---

**CALCulate<cnum>:MARKer<mkr>:X <num>**

(Read-Write) Sets the marker's X-axis value (frequency, power, or time). If the marker is set as delta, the SET and QUERY data is relative to the reference marker. **Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.

<num> Any X-axis position within the measurement span of the marker.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
CALC:MARK:X 100Mhz
calculate2:marker8:x maximum
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:X?

**Return Type** Numeric

**Overlapped?** No

**Default** First Marker turns ON in the middle of the X-axis span. Subsequent markers turn ON at the position of the active marker.

---

## CALCulate<cnum>:MARKer<mkr>:Y?

(Read-only) Reads the marker's Y-axis value. The format of the value depends on the current CALC:MARKER:FORMAT setting. If the marker is set as delta, the data is relative to the reference marker. The query always returns two numbers:

- Smith and Polar formats - (Real, Imaginary)
- LINPhase and LOGPhase - (Real, Imaginary)
- All other formats - (Value,0)

### Critical Note:

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<mkr> Any marker number from 1 to 10; if unspecified, value is set to 1.

#### Examples

```
CALC:MARK:Y?
calculate2:marker3:y?
```

**Query Syntax** CALCulate<cnum>:MARKer<mkr>:Y?

**Return Type** Numeric

**Overlapped?** No


**Default** Not applicable

---

## Calculate:Math Commands

---

Controls math operations on the currently selected measurement and memory.



- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Math Operations](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

### CALCulate<cnum>:MATH:FUNction <char>

(Read-Write) Sets math operations on the currently selected measurement and the trace stored in memory. (There MUST be a trace stored in Memory. See [CALC:MATH MEM](#)) **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<char> The math operation to be applied. Choose from the following:

|                 |                 |
|-----------------|-----------------|
| <b>NORMal</b>   | Trace data only |
| <b>ADD</b>      | Data + Memory   |
| <b>SUBTract</b> | Data - Memory   |
| <b>MULTiPLY</b> | Data * Memory   |
| <b>DIVide</b>   | Data / Memory   |

#### Examples

```
CALC:MATH:FUNC NORM
calculate2:math:function subtract
```

**Query Syntax** CALCulate<cnum>:MATH:FUNction?

**Return Type** Character

**Overlapped?** No

**Default** NORMal

### CALCulate<cnum>:MATH:MEMorize

(Write-only) Puts the currently selected measurement trace into memory. (Data-> Memory) **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

**Examples**

```
CALC:MATH:MEM
calculate2:math:memorize
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

## Calculate:Mixer Command

---

### CALCulate<ch>:MIXer:XAXis <char>

(Read-Write) Sets or returns the swept parameter to display on the X-axis for the selected FCA measurement. [Learn more about X-axis display.](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

#### Parameters

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <char> Parameter to display on the X-axis. Choose from:
- INPUT** - Input frequency span
  - OUTPUT** - Output frequency span
  - LO\_1** - First LO frequency span
  - LO\_2** - Second LO frequency span

#### Examples

```
CALC:MIX:XAX INPUT
calc2:mixer:xaxis output
```

See an example that creates, selects, and calibrates an [SMC](#) and [VMC](#) measurement using SCPI.

**Query Syntax** CALCulate<ch>:MIXer:XAXis?

**Return Type** Character

**Overlapped?** No

**Default** OUTPUT




## Calculate:Normalize Commands

---

Specifies the normalization features used for a receiver power calibration.

**These commands are OBSOLETE (Sept 2004).**

See a new [Receiver Power Cal example](#).

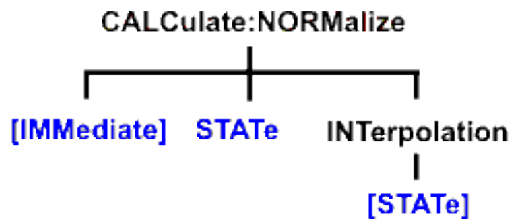

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Receiver Cal](#)

Save and recall your receiver power calibration (which use .CST file commands):

- [SENS:CORR:CSET:SAVE](#)
- [SENS:CORR:CSET\[:SEL\]](#)

Or use these two commands and specify either .STA or .CST file extensions:

- [MMEM:LOAD](#)
- [MMEM:STOR](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---



**CALCulate<cnum>:NORMAlize[:IMMEDIATE] OBSOLETE**

(Write only) This command is replaced with SENS:CORR:COLL:METH RPOWER and SENS:CORR:COLL[:ACQ] POWER

See an example of a Receiver Power Calibration.

Stores the selected measurement's data to that measurement's "divisor" buffer for use by the Normalization data processing algorithm. This command is not compatible with ratioed measurements such as S-parameters. It is intended for receiver power calibration when the selected measurement is of an unratioed power type. Critical Note:

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

**Examples**

```
CALC:NORM
calculate1:normalize:immediate
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**CALCulate<num>:NORMalize:STATe <ON | OFF> OBSOLETE**

(Read-Write) This command is replaced with SENS:CORR[:STATe]ON|OFF

Specifies whether or not normalization is applied to the measurement. Normalization is enabled only for measurements of unratioed power where it serves as a receiver power calibration. Critical Note:

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<ON | OFF> **ON (or 1)** - normalization is applied to the measurement.  
**OFF (or 0)** – normalization is NOT applied to the measurement.

**Examples**

```
CALC:NORM:STAT ON
calculate2:normalize:state off
```

**Query Syntax** CALCulate<num>:NORMalize:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**CALCulate<num>:NORMalize:INTerpolate[:STATe] <ON | OFF> OBSOLETE**

(Read-Write) This command is replaced with SENS:CORR:INT[:STATE]ON|OFF

Turns normalization interpolation ON or OFF. Normalization is enabled only for measurements of unratiod power, where it serves as a receiver power calibration. Critical Note:

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<ON | OFF> **ON (or 1)** – turns interpolation ON.  
**OFF (or 0)** – turns interpolation OFF.

**Examples**

```
CALC:NORM:INT ON
calculate2:normalize:interpolate:state off
```

**Query Syntax** CALCulate<cnum>:NORMalize:INTerpolate[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)


**Overlapped?** No

**Default** ON

## Calculate:Offset Commands

---

Allows the data trace magnitude and phase to be offset.

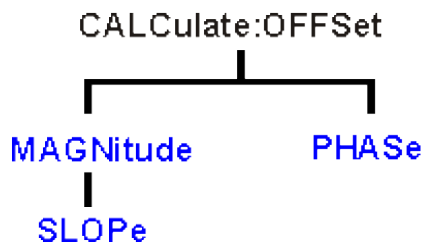

- Click on a blue keyword to view the command details.
- See a [List of all commands](#) in this block.
- [Learn about Magnitude Offset](#)
- [Learn about Phase Offset](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

### CALCulate<cnum>:OFFSet:MAGNitude <num>

(Read-Write) Offsets the data trace magnitude by the specified value.

To offset the data trace magnitude to a slope value that changes with frequency, use [CALC:OFFS:MAGN:SLOP](#)

#### Critical Note

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Offset value in dB.

#### Examples

```
CALC:OFFS:MAGN:4
calculat1:offset:magnitude -2
```

**Query Syntax** CALCulate<cnum>:OFFSet:MAGNitude?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### CALCulate<cnum>:OFFSet:MAGNitude:SLOPe <num>

(Read-Write) Offsets the data trace magnitude to a value that changes linearly with frequency. The offset slope begins at 0 Hz.

**Critical Note**

**Parameters**

- <cnm> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnm> is set to 1.
- <num> Offset slope value in dB/ 1GHz.

**Examples**

```
CALC:OFFS:MAGN:SLOP 1 'Offset slope set to 1dB/GHz
calculat1:offset:magnitude:slope -2 'Offset slope set to -
2dB/GHz
```

**Query Syntax** CALCulate<cnm>:OFFSet:MAGNitude:SLOPe?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**CALCulate<cnm>:OFFSet:PHASe <num>[<char>]**

(Read-Write) Sets the phase offset for the selected measurement. Critical Note:

**Parameters**

- <cnm> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnm> is set to 1.
- <num> Offset phase value. Choose any number between: **-360** and **360**
- <char> Units for phase. OPTIONAL. Choose either:  
**DEG** - Degrees (default)  
**RAD** - Radians

**Examples**

```
CALC:OFFS:PHAS 10
calculate:offset:phase 20rad
```

**Query Syntax** CALCulate:OFFSet:PHASe?

**Return Type** Numeric, returned value always in degrees

**Overlapped?** No


**Default** 0 degrees

---

## Calculate:Parameter Commands

---

Lists, creates, selects and deletes measurements.

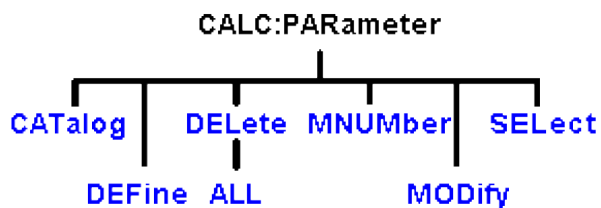

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Measurement Parameters](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using `CALC:PAR:SEL`.

---

### CALCulate<num>:PARAmeter:CATalog?

(Read-only) Returns the names and parameters of existing measurements for the specified channel.

**Note:** For Balanced Measurements: CALC:PAR:CAT? may have an unexpected behavior. [Learn more.](#)

Critical Note:

#### Parameters

<num> Channel number of the measurements to be listed. If unspecified, <num> is set to 1.

#### Examples

```
CALC:PAR:CAT?
calculate2:parameter:catalog?
```



**Return Type** String - "<measurement name>,<parameter>,<measurement name>,<parameter>..."

**Overlapped?** No

**Default** "CH1\_S11\_1,S11"

---

### CALCulate<num>:PARAmeter:DEFine <Mname>,<param>[,port]

(Write-only) Creates a measurement but does NOT display it.

There is no limit to the number of measurements that can be created. However, there is a limit to the number of measurements that can be displayed. See [Traces, Channels, and Windows on the PNA](#).

- Use `DISP:WIND:STATe` to create a window if it doesn't already exist.
- Use `DISP:WIND<wnum>:TRAC<tnum>:FEED <Mname>` to display the measurement.

You must select the measurement (`CALC<cnum>:PAR:SEL <mname>`) before making additional settings.

**Critical Note:**

**Parameters**

<cnum> Channel number of the new measurement. If unspecified, value is set to 1.

<Mname> Name of the measurement. Any non-empty, unique string, enclosed in quotes.

<param> **For S-parameters:**

Any S-parameter available in the PNA

For example: S21

**For ratioed measurements:**

Any two receivers that are available in the PNA. (See the [block diagram](#) showing the receivers in YOUR PNA.)

For example: AR1

**For non-ratioed measurements:**

Any receiver that is available in the PNA. (See the [block diagram](#) showing the receivers in YOUR PNA.)

For example: A

**For Balanced Measurements:**

First create an S-parameter measurement, then change the measurement using `CALC:FSIM:BAL` commands. [See an example](#).

[port] Optional argument;

For multi-port reflection S-parameter measurements: specifies the PNA port which will provide the load for the calibration. This argument is ignored if a transmission S-parameter is specified.

For all non S-parameter measurements: specifies the source port for the measurement.

**Examples** `CALC4:PAR:DEF 'ch4_s33',s33,2 'Defines an S33 measurement with a load on port2 of the analyzer.`

`calculate2:parameter:define 'ch1_a', a, 1 'unratioed meas`

`calculate2:parameter:define 'ch1_a', ar1,1 'ratioed meas`

**Query Syntax** Not Applicable; see [Calc:Par:Cat?](#)

**Overlapped?** No

Default Not Applicable

---

### **CALCulate<cnum>:PARAmeter:DELeTe [:NAME]<Mname>**

(Write-only) Deletes the specified measurement. Critical Note:

#### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<Mname> String - Name of the measurement

**Examples** `CALC:PAR:DEL 'TEST'`  
`calculate2:parameter:delete 'test'`

**Query Syntax** Not Applicable

Overlapped? No

Default Not Applicable

---

### **CALCulate:PARAmeter:DELeTe:ALL**

(Write-only) Deletes all measurements on the PNA. Critical Note:

#### **Parameters**

**Examples** `CALC:PAR:DEL:ALL`

**Query Syntax** Not Applicable

Overlapped? No

Default Not Applicable

---

### **CALCulate<cnum>:PARAmeter:MNUMBER?**



(Read-only) Returns the measurement number of the selected measurement. This is useful when needing to identify a measurement by number, such as with Status:Ques:Lim or Status:Oper:Aver commands. **Critical Note:**

**Parameters**

<cnnum> Channel number of the measurement. If unspecified, <cnnum> is set to 1.

**Examples** `CALC:PAR:MNUM?`  
`calculate2:parameter:mnumber?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**CALCulate<cnnum>:PARAmeter:MODify <param>**

(Write-only) Modifies a standard measurement using the same arguments as CALC:PAR:DEF. To modify an FCA measurement, use CALC:CUST:MOD. **Critical Note:**

**Parameters**

<cnnum> Channel number of the measurement. The selected measurement on that channel will be changed. If unspecified, <cnnum> is set to 1.

<param> Measurement parameter to change to. Use the same <param> arguments as CALC:PAR:DEF.

**Examples** `SYST:PRESET`  
`CALC:PAR:DEF "MyMeas", S11`  
`CALC:PAR:SEL "MyMeas"`  
`CALC:PAR:MOD AR1 'changes the selected S11 measurement to an A/R1 measurement`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**CALCulate<cnnum>:PARAmeter:SELEct <Mname>**

(Read-Write) Sets the selected measurement. Most CALC: commands require that this command be sent before a setting change is made. One measurement on each channel can be selected at the same time. To obtain a list of currently named measurements, use CALC:PAR:CAT? **Critical Note:**

**Parameters**

- <num> Channel number of the measurement to be selected. If unspecified, <num> is set to 1.
- <Mname> String - Name of the measurement. (Do NOT include the parameter name.)

**Examples**

```
CALC:PAR:SEL 'TEST'
calculate2:parameter:select 'test'
```

**Query Syntax** CALCulate:PARameter:SElect?

**Return Type** String

**Overlapped?** No

**Default** The preset measurement name is "CH1\_S11\_1"

## Calculate:RData? Command

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

### CALCulate<cnum>:RDATA? <char>

(Read-only) Returns receiver data for the selected measurement. To query measurement data, see [CALC:DATA?](#)

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<char> Choose from receivers:

**A**

**B**

**R1**

**R2**

**REF** - returns either R1 or R2 data depending on the source port of the CALC-selected measurement.

#### Example

```
GPIB.Write "INITiate:CONTinuous OFF"
GPIB.Write "INITiate:IMMediate;*wai"
GPIB.Write "CALCulate:RDATA? A"
```

**Return Type** Depends on [FORM:DATA](#) - Two numbers per data point

**Overlapped?** No

**Default** Not Applicable

#### Notes:

Generally when you query the analyzer for data, you expect that the number of data values returned will be consistent with the number of points in the sweep.

However, if you query **receiver** data while the instrument is sweeping, the returned values may contain zeros. For example, if your request for receiver data is handled on the 45th point of a 201 point sweep, the first 45 values will be valid data, and the remainder will contain complex zero.


This can be avoided by synchronizing this request with the end of a sweep or putting the channel in hold mode.

[Learn about Unratioed Measurements](#)

## Calculate:Smoothing Commands

---

Controls point-to-point smoothing. Smoothing is a noise reduction technique that averages adjacent data points in a measurement trace. Choose the amount of smoothing by specifying either the number of points or the aperture. Smoothing is not the same as CALC:AVERage which averages each data point over a number of sweeps.

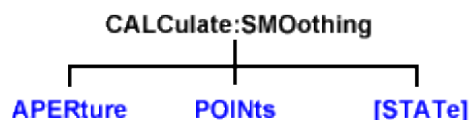

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- See an [example](#) using some of these commands.
- [Learn about Smoothing](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using CALC:PAR:SEL.

---


### CALCulate<cnum>:SMOothing:APERture <num>

(Read-Write) Sets the amount of smoothing as a percentage of the number of data points in the channel. **Critical Note:**

#### Parameters

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <num> Percentage value. Choose any number between: **1 and 25**

#### Examples



```
CALC:SMO:APER 2
calculate2:smoothing:aperture 20.7
```

**Query Syntax** CALCulate<cnum>:SMOothing:APERture?

**Return Type** Numeric

**Overlapped?** No

**Default** 1.5

---

### CALCulate<cnum>:SMOothing:POINTs <num>

(Read-Write) Sets the number of adjacent data points to average. **Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <num> Number of points from 1 point to maximum of 25% of data points in the channel. For example: if number of points in a data trace = 401, the maximum value for points = 100. The points value is always rounded to the closest odd number.

**Examples**

```
CALC:SMO:POIN 50
calculate2:smoothing:points 21
```

**Query Syntax** CALCulate<cnum>:SMOothing:POINTs?

**Return Type** Numeric

**Overlapped?** No

**Default** 3

---

**CALCulate<cnum>:SMOothing[:STATe] <ON | OFF>**

(Read-Write) Turns data smoothing ON or OFF. **Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <ON | OFF> **ON** (or 1) - turns smoothing ON.  
**OFF** (or 0) - turns smoothing OFF.

**Examples**

```
CALC:SMO ON
calculate2:smoothing:state off
```

**Query Syntax** CALCulate<cnum>:SMOothing[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No


**Default** OFF

---

## Calculate:Transform Commands

---

Specifies the settings for time domain transform.

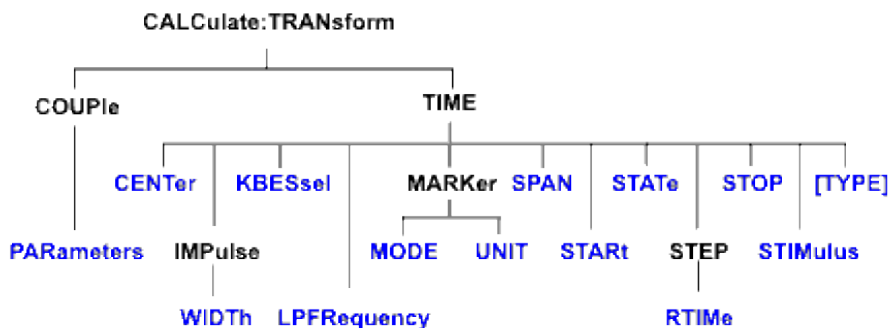

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Time Domain](#)

---

**Note:** CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).

---

### CALCulate<cnm>:TRANSform:COUPlE:PARAmeters <num>

(Read-Write) Specifies the time domain transform parameters to be coupled. The settings for those parameters will be copied from the selected measurement to all other measurements on the channel.

- To turn coupling ON and OFF, use [SENS:COUP:PAR](#)
- To specify Gating parameters to couple, use [CALC:FILT:COUP:PAR](#)

Learn more about [Time Domain Trace Coupling](#)

#### Critical Note:

##### Parameters



- <cnm> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnm> is set to 1.
- <num> (Numeric) Parameters to couple. To specify more than one parameter, add the numbers.
- 1 - Transform Stimulus (Start, Stop, Center, and Span TIME settings.)
  - 2 - Transform State (ON / OFF)
  - 4 - Transform Window (Kaiser Beta / Impulse Width)
  - 8 - Transform Mode (Low Pass Impulse, Low Pass Step, Band Pass)
  - 16 - Transform Distance Marker Units

**Examples** 'To couple all parameters:  
CALC:TRAN:COUP:PAR 31  
'To couple Stimulus and Mode:  
calculate2:transform:couple:parameters 9

**Query Syntax** CALCulate<cnum>:TRANSform:COUPle:PARameters?

**Return Type** Numeric

**Overlapped?** No

**Default** 29 (All parameters except 2 - Transform State)

---

### CALCulate<cnum>:TRANSform:TIME:CENTer <num>

(Read-Write) Sets the center time for time domain measurements. **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Center time in seconds; any number between:  
 $\pm (\text{number of points}-1) / \text{frequency span}$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples** CALC:TRAN:TIME:CENT 1e-8  
calculate2:transform:time:center 15 ps

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:CENTer?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### CALCulate<cnum>:TRANSform:TIME:IMPulse:WIDTh <num>

(Read-Write) Sets the impulse width for the transform window. **Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <num> Impulse width in seconds; Choose any number between: **.6 / frequency span** and **1.39 / frequency span**

**Examples**

```
CALC:TRAN:TIME:IMP:WIDTH 10
calculate2:transform:time:impulse:width 13
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:IMPulse:WIDTH?

**Return Type** Numeric

**Overlapped?** No

**Default** .98 / Default Span

---

**CALCulate<cnum>:TRANSform:TIME:KBESsel <num>**

(Read-Write) Sets the parametric window for the Kaiser Bessel window. **Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <num> Window width for Kaiser Bessel in seconds; Choose any number between: **0.0** and **13.0**

**Examples**

```
CALC:TRAN:TIME:KBES 10
calculate2:transform:time:kbessel 13
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:KBESsel?

**Return Type** Numeric

**Overlapped?** No

**Default** 6

---

**CALCulate<cnum>:TRANSform:TIME:LPFREQuency**



(Write-only) Sets the start frequencies in LowPass Mode. **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

**Examples**

```
CALC:TRAN:TIME:LPFR
calculate2:transform:time:lpfrequency
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**CALCulate<num>:TRANSform:TIME:MARKer:MODE <char>**

(Read-Write) Specifies the measurement type in order to determine the correct marker distance.

- Select Auto for S-Parameter measurements.
- Select Reflection or Transmission for arbitrary ratio or unratiod measurements.

This setting affects the display of ALL markers for only the ACTIVE measurement.

Learn more about [Distance Markers](#).

**Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<char> Choose from:

**AUTO** If the active measurement is an S-Parameter, automatically chooses reflection or transmission. If non S-Parameter measurements, reflection is chosen.

**REFlection** Displays the distance from the source to the receiver divided by two (to compensate for the return trip.)

**TRANsmission** Displays the distance from the source to the receiver.

**Examples**

```
CALC:TRAN:TIME:MARK:MODE REFL
calculate2:transform:time:marker:mode auto
```

**Query Syntax** CALCulate<num>:TRANSform:TIME:MARKer:MODE?

**Return Type** Character

**Overlapped?** No

**Default** Auto

---

## CALCulate<cnum>:TRANSform:TIME:MARKer:UNIT <char>

(Read-Write) Specifies the unit of measure for the display of marker distance values. This settings affects the display of ALL markers for only the ACTIVE measurement (unless Distance Maker Units are coupled using [CALC:TRAN:COUP:PAR](#)).

Learn more about [Distance Markers](#).

### Critical Note:

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<char> Choose from:

**METRs**

**FEET**

**INCHes**

#### Examples

```
CALC:TRAN:TIME:MARK:UNIT INCH
calculate2:transform:time:marker:unit feet
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:MARKer:UNIT?

**Return Type** Character

**Overlapped?** No

**Default** METRs

---

## CALCulate<cnum>:TRANSform:TIME:SPAN <num>

(Read-Write) Sets the span time for time domain measurements. **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Span time in seconds; any number between:  
**0** and  $2 * [(number\ of\ points - 1) / frequency\ span]$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

#### Examples

```
CALC:TRAN:TIME:SPAN 1e-8
calculate2:transform:time:span maximum
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:SPAN?

**Return Type** Numeric

**Overlapped?** No

**Default** 20 ns

---

### CALCulate<cnum>:TRANSform:TIME:STARt <num>

(Read-Write) Sets the start time for time domain measurements. **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Start time in seconds; any number between:  
 $\pm (\text{number of points}-1) / \text{frequency span}$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

#### Examples

```
CALC:TRAN:TIME:STAR 1e-8
calculate2:transform:time:start minimum
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:STARt?

**Return Type** Numeric

**Overlapped?** No

**Default** -10 ns

---

### CALCulate<cnum>:TRANSform:TIME:STATe <ON | OFF>

(Read-Write) Turns the time domain transform capability ON or OFF. **Critical Note:**

**Note:** Sweep type must be set to Linear Frequency in order to use Time Domain Transform.

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<ON|OFF> **ON** (or 1) - turns time domain ON.  
**OFF** (or 0) - turns time domain OFF.

#### Examples

```
CALC:TRAN:TIME:STAT ON
calculate2:transform:time:state off
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

## CALCulate<cnum>:TRANSform:TIME:STOP <num>

(Read-Write) Sets the stop time for time domain measurements. **Critical Note:**

### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Stop time in seconds; any number between:  
 $\pm (\text{number of points}-1) / \text{frequency span}$

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

### Examples

```
CALC:TRAN:TIME:STOP 1e-8
calculate2:transform:time:stop maximum
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:STOP?

**Return Type** Numeric

**Overlapped?** No

**Default** 10 ns

---

## CALCulate<cnum>:TRANSform:TIME:STEP:RTIME <num>

(Read-Write) Sets the step rise time for the transform window. **Critical Note:**

### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<num> Rise time in seconds; Choose any number between:  
**.45 / frequency span** and **1.48 / frequency span**

### Examples

```
CALC:TRAN:TIME:STEP:RTIM 1e-8
calculate2:transform:time:step:runtime 15 ps
```

**Query Syntax** CALCulate<cnum>:TRANSform:TIME:STEP:RTIME?

**Return Type** Numeric

**Overlapped?** No

**Default** .99 / Default Span

---

## CALCulate<cnum>:TRANSform:TIME:STIMulus <char>

(Read-Write) Sets the type of simulated stimulus that will be incident on the DUT. **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<char> Choose from:  
**STEP** - simulates a step DUT stimulus  
**IMPulse** - simulates a pulse DUT stimulus

---

STEP can ONLY be used when CALC:TRAN:TIME:TYPE is set to LPASs (Lowpass).  
(STEP **cannot** be used with TYPE = BPASs.)

---

:STIM **STEP** will set :TYPE to **LPASs**

:TYPE **BPASs** will set :STIM to **IMPulse**

**Examples**

```
CALC:TRAN:TIME:STIM STEP
calculate2:transform:time:stimulus impulse
```

**Query Syntax** CALCulate<num>:TRANSform:TIME:STIMulus?

**Return Type** Character

**Overlapped?** No

**Default** IMPulse

---

**CALCulate<num>:TRANSform:TIME[:TYPE] <char>**

(Read-Write) Sets the type of time domain measurement. **Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<char> Type of measurement. Choose from:  
**LPASs** - Lowpass; Must also send CALC:TRAN:TIME:LPFRequency before calibrating.  
**BPASs** - Bandpass;

---

BPASs can **only** be used when CALC:TRAN:TIME:STIM is set to IMPulse. (BPASs **cannot** be used with :STIM = STEP)

---

:STIM **STEP** will set :TYPE to **LPASs**

:TYPE **BPASs** will set :STIM to **IMPulse**

**Examples**

```
CALC:TRAN:TIME LPAS
calculate2:transform:time:type bpas
```

**Query Syntax** CALCulate<num>:TRANSform:TIME[:TYPE]?

**Return Type** Character


**Overlapped?** No



## Control Commands

---

Specifies the settings to remotely control the rear panel connectors and ECAL Module state.

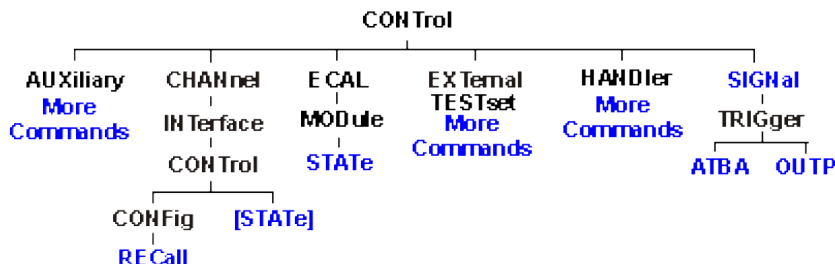

- Click on a **blue** keyword to view the command details.
  - See a [List](#) of all SCPI commands.
  - See a pinout and detailed description of the rear panel connectors:
    - [Auxilliary IO connector](#)
    - [External Test Set IO connector](#)
    - [Material Handler IO connector](#)
- 

### CONTROL:CHANnel:INTerface:CONTRol:CONFig:RECall <string>

(Write-only) Recalls an Interface Control configuration file. [Learn more about Interface Control.](#)

#### Parameters

<string> File name and extension (.xml) of the configuration file to recall. Files are typically stored in the default folder "C:\Program Files\Agilent\Network Analyzer\Documents". To recall from a different folder, specify the full path name.



#### Examples

```
CONTROL:CHAN:INT:CONT:CONF:REC 'MyConfigFile.xml'
control:channel:interface:control:config:recall 'C:\Program
Files\Agilent\Network Analyzer\Documents\MyFile.xml'
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### CONTROL:CHANnel:INTerface:CONTRol[:STATe] <bool>

(Read-Write) Enables and disables ALL Interface Control settings. To send data, the individual interfaces must also be enabled. [Learn more about Interface Control.](#)

**Parameters**

<bool> Boolean  
**False (0)** - Interface Control is disabled;NO control data is sent.  
**True (1)** - Interface Control is enabled.

**Examples** `CONT:CHAN:INT:CONT 1`  
`control:channel:interface:control:state 0`

**Query Syntax** `CONTrol:CHANnel:INTerface:CONTrol[:STATe]?`

**Return Type** Boolean

**Overlapped?** No

**Default** False (0)

**CONTrol:ECAL:MODule[num]:STATe <value>**

(Write-only) Sets the internal state of the selected ECAL module.

**Parameters**

[num] Optional argument. USB number of the ECal module. If unspecified (only one ECal module is connected to the USB), <num> is set to 1. If two or more modules are connected, use [SENS:CORR:COLL:CKIT:INF?](#) to verify their identity.

<value> Integer code for switching the module. The following are codes for Agilent ECal modules.

| Agilent 8509x Modules |        |        |
|-----------------------|--------|--------|
| State                 | Port A | Port B |
| Open                  | 0      | 0      |
| Short                 | 43     | 43     |
| Load                  | 33     | 33     |
| Mismatch              | 4      | 16     |
| Thru                  | 84     |        |
| Confidence            | 20     |        |



| <b>Agilent N469x Modules</b>  |               |               |
|-------------------------------|---------------|---------------|
| <b>State</b>                  | <b>Port A</b> | <b>Port B</b> |
| Open                          | 36            | 33            |
| Short                         | 39            | 45            |
| Load                          | 37            | 37            |
| Mismatch<br>(Offset short)    | 53            | 53            |
| Impedance 5<br>(Offset open)  | 5             | 5             |
| Impedance 6<br>(Offset short) | 21            | 21            |
| Impedance 7<br>(Offset short) | 38            | 41            |
| Thru                          | 42            |               |
| Confidence                    | 40            |               |

| <b>Agilent N4431 Modules</b> |               |               |               |               |
|------------------------------|---------------|---------------|---------------|---------------|
| <b>State</b>                 | <b>Port A</b> | <b>Port B</b> | <b>Port C</b> | <b>Port D</b> |
| Open                         | -1398         | -1384         | -2774         | -2654         |
| Short                        | -1350         | -1381         | -2582         | -2642         |
| Load                         | 26985         | -26986        | -26986        | 26985         |
| Mismatch                     | -26986        | 26985         | 26985         | -26986        |

| Path    | Thru  | Confidence |
|---------|-------|------------|
| AB Path | -2590 | -598       |
| AC Path | -4011 | 85         |
| AD Path | -2517 | 16042      |
| BC Path | -1650 | -598       |
| BD Path | -4011 | 85         |
| CD Path | -1352 | 16042      |

**Examples** `CONT:ECAL:MOD:STAT 36`  
`control:ecal:module2:state 38`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

## CONTrol:SIGNal <conn>,<char>

(Read-Write) Configures external triggering in the PNA.

Trigger:Sequence:Source is automatically set to External when **CONTrol:SIGNal** is sent.

Edge triggering is only available on some Microwave PNA models.

For more information, see External Triggering in the PNA.

### Parameters

<conn> Rear Panel connector to send or receive trigger signals. Choose from:

**BNC1** Trigger IN from rear-panel Trigger IN BNC connector

**AUXT** Trigger IN from AUX IO connector Pin 19

---

**Note:** Only one of the input connectors is active at a time. When a command is sent to one, the PNA automatically makes the other INACTIVE.

---

**BNC2** Trigger OUT to rear-panel Trigger OUT BNC connector.

**MATHtrigger** - Trigger IN from rear-panel Material Handler connector Pin 18

<char> **INACTIVE** - Disables the specified connector <conn>.

**Choose from ONLY the following** when <conn> is set to either **BNC1** or **AUXT**:

**TIENEGATIVE** - (Trigger In Edge Negative) - Triggers the PNA when receiving a negative going signal

**TIEPOSITIVE** - (Trigger In Edge Positive) - Triggers the PNA when receiving a positive going signal

**TILLOW** - (Trigger In Level Low) - Triggers the PNA when receiving a low level signal

**TILHIGH** - (Trigger In Level High) - Triggers the PNA when receiving a High-level signal

**Choose from ONLY the following** when <conn> is set to **BNC2**:

Use CONTROL:SIGNal:TRIGger:OUTP to enable the BNC2 output.

**TOPPAFTER** - (Trigger Out Pulse Positive After) - Sends a POSITIVE going TTL pulse at the END of each point during the sweep.

**TOPPBEFORE** - (Trigger Out Pulse Positive Before) - Sends a POSITIVE going TTL pulse at the START of each point during the sweep.

**TOPNAFTER** - (Trigger Out Pulse Negative After) - Sends a NEGATIVE going TTL pulse at the END of each point during the sweep.

**TOPNBEFORE** - (Trigger Out Pulse Negative Before) - Sends a NEGATIVE going TTL pulse at the START of each point during the sweep.

**Examples**

```
CONT:SIGN BNC1, TIENEGATIVE
control:signal bnc2, toppbefore
```

**Query Syntax**

CONTROL:SIGNal? <conn>

In addition to the arguments listed above, the following is also a possible returned value:

**NAVAILABLE** - This feature is not available on this PNA

**Return Type**

Character

**Overlapped?**

No

**Default**

At Preset:

BNC1 = INACTIVE

BNC2 = INACTIVE

AUXT = TILHIGH

When Output is enabled:

BNC1 = INACTIVE

BNC2 = TOPPAFTER

AUXT = TILHIGH

---

**CONTROL:SIGNal:TRIGger:ATBA <bool>**

(Read-Write) **Accept Trigger Before Armed** Determines what happens to an EDGE trigger signal if it occurs before the PNA is ready to be triggered. (LEVEL trigger signals are always ignored.) For more information, see [External triggering](#).

#### Parameters

<bool> Boolean  
False (0) - A trigger signal is ignored if it occurs before the PNA is ready to be triggered.  
True (1) - A trigger signal is remembered and then used when the PNA becomes armed (ready to be triggered). The PNA remembers only one trigger signal.

**Examples** `CONT:SIGN:TRIG:ATBA 0`  
`control:signal:trigger:atba true`

**Query Syntax** `CONTrol:SIGNal:TRIGger:ATBA?`

**Return Type** Boolean

**Overlapped?** No

**Default** False

---

### **CONTrol:SIGNal:TRIGger:OUTP <bool>**

(Read-Write) **Output Enabled** The PNA can be enabled to send trigger signals out the rear-panel [TRIGGER OUT BNC](#) connector. Use [CONTrol:SIGNal](#) to configure for output triggers.

For more information, see [External triggering](#).

#### Parameters

<bool> Boolean  
False (0) - PNA does NOT output trigger signals.  
True (1) - PNA DOES output trigger signals.

**Examples** `CONT:SIGN:TRIG:OUTP 1`  
`control:signal:trigger:outp false`

**Query Syntax** `CONTrol:SIGNal:TRIGger:OUTP?`

**Return Type** Boolean


**Overlapped?** No

**Default** False

## Display Commands

---

Controls the settings of the front panel screen.

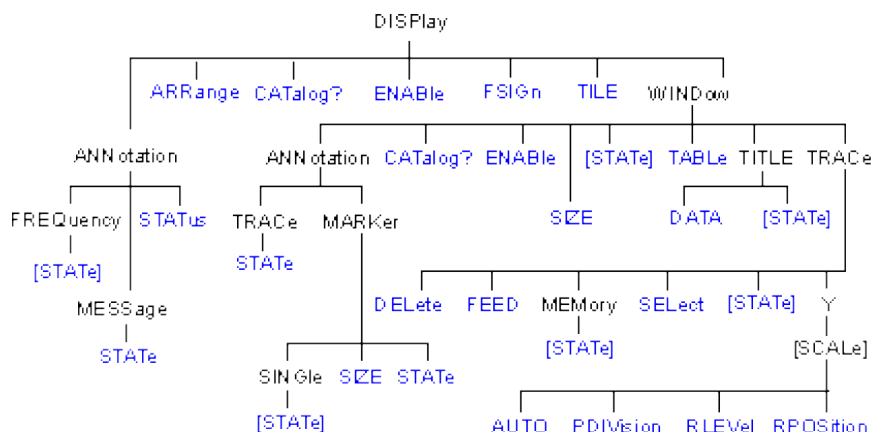

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - See an [example](#) using some of these commands
  - [Learn about Screen Setup](#)
- 

### DISPlay:ANNOtation:FREQUency[:STATe] <ON | OFF>

(Read-Write) Turns frequency information on the display title bar ON or OFF for all windows.

#### Parameters

<ON | OFF> **ON** (or 1) - turns frequency annotation ON.  
**OFF** (or 0) - turns frequency annotation OFF.



#### Examples

```
DISP:ANN:FREQ ON
display:annotation:frequency:state off
```

**Query Syntax** DISPlay:ANNOtation:FREQUency[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON (1)

---

### DISPlay:ANNOtation:MESSAge:STATe <ON | OFF>

(Read-Write) Enables and disables error pop-up messages on the display.

**Parameters**

<ON | OFF> **ON** (or 1) - enables error pop-up messages  
**OFF** (or 0) - disables error pop-up messages

**Examples**

```
DISP:ANN:MESS:STAT ON
display:annotation:message:state off
```

**Query Syntax** DISPlay:ANNotation:MESSage:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON (1)

---

**DISPlay:ANNotation:STATus <ON | OFF>**

(Read-Write) Turns the status bar at the bottom of the screen ON or OFF. The status bar displays information for the active window.

**Parameters**

<ON | OFF> **ON** (or 1) - turns status bar ON.  
**OFF** (or 0) - turns status bar OFF.

**Examples**

```
DISP:ANN:STAT ON
display:annotation:status off
```

**Query Syntax** DISPlay:ANNotation:STATus?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** Last state that was set

---

**DISPlay:ARRange <char>**

(Read-Write) Places EXISTING measurements into pre-configured window arrangements. Overlay, Stack(2), Split(3), and Quad(4) creates new windows. To learn more, see [Arrange Existing Measurements](#).

### Parameters

<char> Window arrangement. Choose from:

- TILE - tiles existing windows
- CASCade - overlaps existing windows
- OVERlay - all traces placed in 1 window
- STACk - 2 windows
- SPLit - 3 windows
- QUAD - 4 windows

**Examples** `DISP:ARR CASC`  
`display:arrange cascade`

**Query Syntax** DISPLAY:ARRange?

**Return Type** Character

**Overlapped?** No

**Default** TILE

---

### DISPlay:CATalog?

(Read-only) Returns the existing Window numbers.

**Return Type** String of Character values, separated by commas

**Example** Two windows with numbers 1 and 2 returns:  
"1,2"

**Overlapped?** No

**Default** Not applicable

---

### DISPlay:ENABLE <ON | OFF>

(Read-Write) Specifies whether to disable or enable all analyzer display information **in all windows** in the analyzer application. Marker data is not updated. More CPU time is spent making measurements instead of updating the display.

**Parameters**

<ON | OFF> **ON** (or 1) - turns the display ON.  
**OFF** (or 0) - turns the display OFF.

**Examples** `DISP:ENAB ON`  
`display:enable off`

**Query Syntax** DISPlay:ENABLE?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

**DISPlay:FSIGN <ON | OFF>**

(Read-Write) Shows or hides the window which displays global pass/fail results.

**Parameters**

<ON | OFF> **ON** (or 1) - displays the pass/fail dialog  
**OFF** (or 0) - hides the pass/fail dialog

**Examples** `DISP:FSIG ON`  
`display:fsign off`

**Query Syntax** DISPlay:FSIGN?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**DISPlay[:TILE] - OBSOLETE - Use DISP:ARRange**

(Write-only) Tiles the windows on the screen.

**Examples** `DISP`  
`display:tile`

**Overlapped?** No

**Default** Not Applicable

---



## DISPlay:WINDow<wnum>:ANNotation:MARKer:SINGle[:STATe] <bool>

(Read-Write) Either shows marker readout of only the active trace or other traces simultaneously.

See other SCPI [Marker](#) commands. Learn more about [Marker readout](#).

### Parameters

- <wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.
- <bool> **ON** (or 1) - Shows the readout of only the active marker for each trace.  
**OFF** (or 0) - Shows up to 5 marker readouts per trace, up to 20 total readouts.

### Examples

```
DISP:WIND:ANN:MARK:SING ON
display:window:annotation:marker:single off
```

**Query Syntax** DISPlay:WINDow:ANNotation:MARKer:SINGle?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

## DISPlay:WINDow<wnum>:ANNotation:MARKer:SIZE <char>

(Read-Write) Specifies the size of the marker readout text. See other SCPI [Marker](#) commands. Learn more about [Marker readout](#).

### Parameters

- <wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.
- <char> Readout text size. Choose from:**NORMAL** | **LARGE**

### Examples

```
DISP:WIND:ANN:MARK:SIZE LARG
display:window:annotation:marker:size normal
```

**Query Syntax** DISPlay:WINDow:ANNotation:MARKer:SIZE?

**Return Type** Character

**Overlapped?** No

**Default** NORMAl

---

## DISPlay:WINDow<wnum>:ANNotation:MARKer:STATe <ON | OFF>

(Read-Write) Specifies whether to show or hide the Marker readout (when markers are ON) on the selected window. See other SCPI [Marker](#) commands. Learn more about [Marker readout](#).

#### Parameters

- <wnum> Any existing window number (**1 to 16**); if unspecified, value is set to 1.
- <ON | OFF> **ON** (or 1) - turns marker readout ON.  
**OFF** (or 0) - turns marker readout OFF.

#### Examples

```
DISP:WIND:ANN:MARK:STAT ON
display:window:annotation:marker:state off
```

**Query Syntax** DISPlay:WINDow:ANNotation:MARKer:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

### DISPlay:WINDow<wnum>:ANNotation:TRACe:STATe <ON | OFF>

(Read-Write) Specifies whether to show or hide the Trace Status buttons on the left of the display.

#### Parameters

- <wnum> Any existing window number (**1 to 16**); if unspecified, value is set to 1.
- <ON | OFF> **ON** (or 1) - turns the buttons ON.  
**OFF** (or 0) - turns the buttons OFF.

#### Examples

```
DISP:WIND:ANN:TRAC:STAT ON
display:window:annotation:trace:state off
```

**Query Syntax** DISPlay:WINDow:ANNotation:TRACe:STATe?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

### DISPlay:WINDow<wnum>:CATalog?

(Read-only) Returns the trace numbers for the specified window.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.

**Example** Window 1 with four traces:  
`DISPlay:WINDow1:CATalog?`  
Returns:  
`"1,2,3,4"`

**Return Type** String of Character values separated by commas

**Overlapped?** No

**Default** Not applicable

---

**DISPlay:WINDow<wnum>:ENABLE <ON | OFF>**

(Read-Write) Specifies whether to disable or enable all analyzer display information **in the specified window**. Marker data is not updated. More CPU time is spent making measurements instead of updating the display.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.

<ON | OFF> **ON** (or 1) - turns the display ON.  
**OFF** (or 0) - turns the display OFF.

**Examples** `DISP:WIND:ENABLE ON`  
`display:window1:enable off`

**Query Syntax** DISPlay:WINDow<wnum>:ENABLE?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

**DISPlay:WINDow<wnum>:SIZE <char>**

(Read-Write) Sets or returns the window setting of Maximized, Minimized, or Normal. To arrange all of the windows, use DISP:ARR.

**Parameters**

<wnum> Any existing window number (**1 to 16**); if unspecified, value is set to 1

<char> Window size. Choose from:

**MIN | MAX | NORM**

**Examples** `DISP:WIND:SIZE MAX`  
`display:window:size norm`

**Query Syntax** `DISPlay:WINDow:SIZE?`

**Overlapped?** No

**Default** Not Applicable

---

**DISPlay:WINDow<wnum>[:STATe] <ON | OFF>**

(Read-Write) Write to create or delete a window on the screen or Read whether a window is present.

**Parameters**

<wnum> Window number to create; choose any integer between:  
**1 and 16**

<ON | OFF> **ON** (or 1) - The window <wnum> is created.  
**OFF** (or 0) - The window <wnum> is deleted.

**Examples** `DISP:WIND ON`  
`display:window2:state off`

**Query Syntax** `DISPlay:WINDow<wnum>[:STATe]?`

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** Window number "1" **ON**

---

**DISPlay:WINDow<wnum>:TABLE <char>**

(Read-Write) Write to show the specified table at the bottom of the analyzer screen or Read to determine what table is visible.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1

<char> Table to show. Choose from:  
**OFF | MARKer | LIMit | SEGMENT**

**Examples** `DISP:WIND:TABLE SEGM`  
`display:window:table off`

**Query Syntax** `DISPlay:WINDow:TABLE?`

**Overlapped?** No

**Default** OFF

---

**DISPlay:WINDow<wnum>:TITLe:DATA <string>**

(Read-Write) Sets data in the window title area. The title is turned ON and OFF with `DISP:WIND:TITL:STAT OFF`.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.

<string> Title to be displayed. Any characters, enclosed with quotes. If the title string exceeds 50 characters, an error will be generated and the title not accepted. Newer entries replace (not append) older entries.

**Examples** `DISP:WIND:TITL:DATA 'hello'`  
`display:window2:title:data 'hello'`

**Query Syntax** `DISPlay:WINDow<wnum>:TITLe:DATA?`

**Return Type** String

**Overlapped?** No

**Default** NA

---

**DISPlay:WINDow<wnum>:TITLe[:STATe] <ON | OFF>**

(Read-Write) Turns display of the title string ON or OFF. When OFF, the string remains, ready to be redisplayed when turned back ON.

**Parameters**

<wnum> Any existing window number (**1 to 16**); if unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns the title string ON.  
**OFF** (or 0) - turns the title string OFF.

**Examples**

```
DISP:WIND:TITL ON
Display:window1:title:state off
```

**Query Syntax** DISPlay:WINDow<wnum>:TITLe[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

**DISPlay:WINDow<wnum>:TRACe<tnum>:DELeTe**

(Write-only) Deletes the specified trace from the specified window. The measurement parameter associated with the trace is not deleted.

**Parameters**

<wnum> Any existing window number (**1 to 16**); if unspecified, value is set to 1.

<tnum> The number of the trace to be deleted; if unspecified, value is set to 1

**Examples**

```
DISP:WIND:TRAC:DEL
display:window2:trace2:delete
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** NA

---

**DISPlay:WINDow<wnum>:TRACe<tnum>:FEED <name>**

(Write-only) Creates a new trace <tnum> and associates (feeds) a measurement <name> to the specified window<wnum>. This command should be executed immediately after creating a new measurement with CALC:PAR:DEF<name>,<parameter>.

To feed the same measurement to multiple traces, create another measurement with the same <name>,<parameter> using the CALC:PAR:DEF command. The analyzer will collect the data only once.

**Parameters**

- <wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.
- <tnum> Trace number to be created. Choose any Integer between 1 and 8
- <name> Name of the measurement that was defined with CALC:PAR:DEF<name>,<parameter>

**Examples**

```
DISP:WIND:TRAC:FEED 'test '
display>window2:trace2:feed 'test '
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** "CH1\_S11"

---

**DISPlay:WINDow<wnum>:TRACe<tnum>MEMory[:STATe] <ON | OFF>**

(Read-Write) Turns the memory trace ON or OFF.

**Parameters**

- <wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.
- <tnum> Any existing trace number; if unspecified, value is set to 1
- <ON | OFF> **ON** (or 1) - turns the memory trace ON.  
**OFF** (or 0) - turns the memory trace OFF.

**Examples**

```
DISP:WIND:TRAC:MEM ON
display>window2:trace2:memory:state off
```

**Query Syntax** DISPlay:WIND<wnum>:TRACe<tnum>:MEMory[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**DISPlay:WINDow<wnum>:TRACe<tnum>:SElect**

(Write-only) Activates the specified trace in the specified window for front panel use.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.

<tnum> Any existing trace number; if unspecified, value is set to 1

**Examples** `DISP:WIND:TRAC:SEL`  
`display:window2:trace2:select`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** NA

---

**DISPlay:WINDow<wnum>:TRACe<tnum>[:STATe] <ON | OFF>**

(Read-Write) Turns the display of the specified trace in the specified window ON or OFF. When OFF, the measurement behind the trace is still active.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.

<tnum> Any existing trace number; if unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns the trace ON.  
**OFF** (or 0) - turns the trace OFF.

**Examples** `DISP:WIND:TRAC ON`  
`display:window2:trace2:state off`

**Query Syntax** DISPlay:WIND<wnum>:TRACe<tnum>[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

**DISPlay:WINDow<wnum>:TRACe<tnum>:Y[:SCALe]:AUTO**



(Write-only) Performs an **Autoscale** on the specified trace in the specified window, providing the best fit display. Autoscale is performed only when the command is sent; it does NOT keep the trace autoscaled indefinitely.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.

<tnum> Any existing trace number; if unspecified, value is set to 1

**Examples**

```
DISP:WIND:TRAC:Y:AUTO
display>window2:trace2:y:scale:auto
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**DISPlay:WINDow<wnum>:TRACe<tnum>:Y[:SCALe]:PDIVision <num>**

(Read-Write) Sets the Y axis **Per Division** value of the specified trace in the specified window.

**Parameters**

<wnum> Any existing window number (1 to 16); if unspecified, value is set to 1.

<tnum> Any existing trace number; if unspecified, value is set to 1

<num> Units / division value. The range of acceptable values is dependent on format and domain.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
DISP:WIND:TRAC:Y:PDIV 1
display>window2:trace2:y:scale:pdivision maximum
```

**Query Syntax** DISPlay:WINDow<wnum>:TRACe<tnum>:Y[:SCALe]:PDIVision?

**Return Type** Numeric

**Overlapped?** No

**Default** 10

---

**DISPlay:WINDow<wnum>:TRACe<tnum>:Y[:SCALe]:RLEVel <num>**

(Read-Write) Sets the Y axis Reference Level of the specified trace in the specified window.

**Parameters**

- <wnum> Any existing window number (**1 to 16**); if unspecified, value is set to 1.
- <tnum> Any existing trace number; if unspecified, value is set to 1
- <num> Reference level value. The range of acceptable values is dependent on format and domain.

---

**Note:** This command will accept MIN or MAX instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
DISP:WIND:TRAC:Y:RLEV 0
display:window2:trace2:y:scale:rlevel minimum
```

**Query Syntax** DISPlay:WINDow<wnum>:TRACe<tnum>:Y[:SCALe]:RLEVel?

**Return Type** Numeric

**Overlapped?** No

**Default** NA

---

**DISPlay:WINDow<wnum>:TRACe<tnum>:Y[:SCALe]:RPOStion <num>**

(Read-Write) Sets the **Reference Position** of the specified trace in the specified window

**Parameters**

- <wnum> Any existing window number (**1 to 16**); if unspecified, value is set to 1.
- <tnum> Any existing trace number; if unspecified, value is set to 1
- <num> Reference position on the screen measured in horizontal graticules from the bottom. The range of acceptable values is dependent on format and domain.

---

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
DISP:WIND:TRAC:Y:RPOS 0
display:window2:trace2:y:rposition maximum
```

**Query Syntax** DISPlay:WINDow<wnum>:TRACe<tnum>:Y[:SCALe]:RPOStion?

**Return Type** Numeric

**Overlapped?** No

**Default** 5


---



## Format Commands

---

Specifies the way that data will be transferred when moving large amounts of data. These commands will affect data that is transferred with the [CALC:DATA](#) and [CALC:RDATA](#) commands.

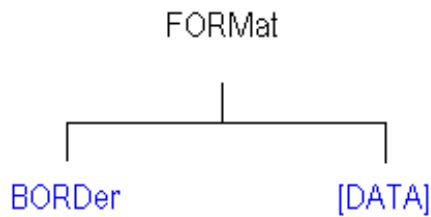

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
- 

### FORMat:BORDER <char>

(Read-Write) Set the byte order used for GPIB data transfer. Some computers read data from the analyzer in the reverse order. This command is only implemented if FORMAT:DATA is set to :REAL. If FORMAT:DATA is set to :ASCII, the swapped command is ignored.

#### Parameters

<char> Choose from:

**NORMAL** - Use when your controller is anything other than an IBM compatible computers

**SWAPPED** - for IBM compatible computers

---

Note: Use **NORMAL** if you are using drivers like VISA or development environments like VEE, LabView, or T&M Tool kit.

---

#### Examples

```
FORM:BORD SWAP
format:border normal
```



**Query Syntax** FORMat:BORDER?

**Return Type** Character

**Overlapped?** No

**Default** Normal

---

### FORMat[:DATA] <char>

(Read-Write) Sets the data format for data transfers. To transfer measurement data, use the CALC:DATA command.

To transfer Source Power correction data, use SOURce:POWer:CORRection:COLLect:TABLE:DATA  
SOURce:POWer:CORRection:COLLect:TABLE:FREQUency  
SOURce:POWer:CORRection:DATA

### Parameters

<char> Choose from:  
**REAL,32** - (default value for REAL) Best for transferring large amounts of measurement data.  
**REAL,64** - Slower but has more significant digits than REAL,32. Use REAL,64 if you have a computer that doesn't support REAL,32.  
**ASCii,0** - The easiest to implement, but very slow. Use if small amounts of data to transfer.  
Note: The **REAL,32** and **REAL,64** arguments transfer data in block format as explained in Transferring Measurement Data.

**Examples** `FORM REAL,64`  
`format:data ascii`

**Query Syntax** FORMat:DATA?

**Return Type** Character,Character

**Overlapped?** No

**Default** ASCii,0

---

## Hardcopy Command

---

[Learn about Printing](#)

### HCOPY:FILE <filename>

(Write-only) Saves the screen image to a file.

#### Parameters

<filename> Name of the file to save the screen to. The file is saved to the current working directory unless a valid full path name is specified.

Use one of the following suffixes:

.bmp - not recommended due to large file size

.jpg - not recommended due to poor quality

.png - recommended

#### Examples

```
HCOPY:FILE "myFile.png"
hcopy:file "c:\data\myfile.png"
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### HCOPY[:IMMEDIATE]

(Write-only) Prints the screen to the default printer.

#### Examples

```
HCOPY
hcopy:immediate
```

**Query Syntax** Not applicable


**Overlapped?** No

**Default** Not Applicable

## Initiate Commands

---

Controls triggering signals



- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Triggering](#)
- 

### INITiate:CONTInuous <boolean>

(Read-Write) Specifies whether the PNA trigger source is set to Internal (continuous) or Manual.

This command is a subset of [TRIG:SEQ:SOURce](#), which can also set the trigger source to External.

To set how a channel responds to trigger signals, use [SENS:SWE:MODE](#).

See a [map of user interface to SCPI triggering commands](#).

For more information on triggering, see the [PNA Trigger Model](#)

#### Parameters

<boolean> **ON** (or 1) - Internal (continuous) trigger.  
**OFF** (or 0) - Manual sweep. Use [INIT:IMMediate](#) to send a trigger signal

#### Examples

```
INIT:CONT ON
initiate:continuous off
```

**Query Syntax** INITiate:CONTInuous?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

### INITiate<num>[:IMMediate]

(Write-only) Stops the current sweeps and immediately sends a trigger to the specified channel. (Same as Sweep \ Trigger \ Trigger! on the PNA front panel).

- If the specified channel is in HOLD, it will sweep one time and return to HOLD when complete.
- If Trigger:Scope = Global, all channels will receive a trigger.
- If Trigger:Scope = Channel (only the active channel receives a trigger) and the specified channel is not the active channel, the specified channel will NOT receive a trigger signal.
- If the specified channel is NOT in Manual trigger (INIT:CONT OFF), the analyzer will return an error.
- If channel <cnun> does not exist, the analyzer will return an error.

---

**Note:** An **SMC Fixed Output** measurement cannot be triggered using this command. For more information, see the [example program](#).

---

### Parameters

<cnun> Any existing channel number. If unspecified, value is set to 1

**Examples** `INIT  
initiate2:immediate`

**Query Syntax** Not applicable

**Overlapped?** Yes

**Default** Not applicable


---



## Memory Commands

---

The memory commands control saving and loading instrument states and measurement trace data to the hard drive. To read and write trace data in GPIB format, see [CALC:DATA](#).

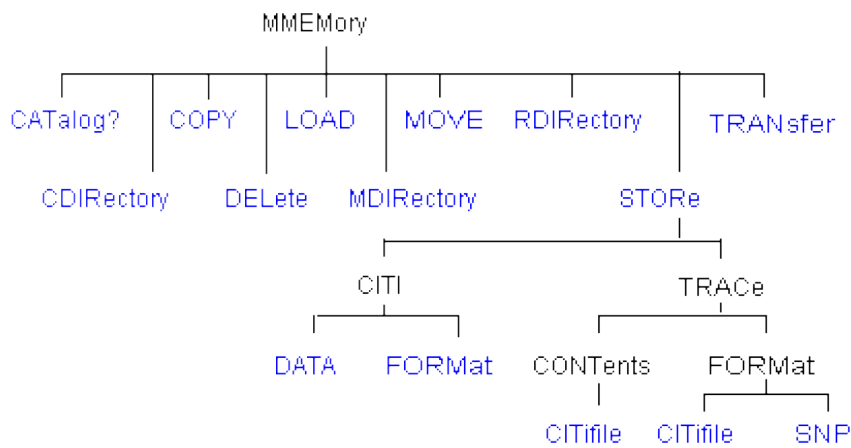

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Save / Recall and File Types](#)

### Specifying Path Names

The MMEM commands use the following rules to specify path names:

- The default folder is "C:\Program Files\Agilent\Network Analyzer\Documents"
- You can change the active directory using [MMEMory:CDIRECTory](#).
- Specify only the file name if using the active directory.
- You can also use an absolute path name to specify the folder and file.



**MMEMory:CATalog[:<char>]? [<folder>]**

(Read-only) Returns a comma-separated string of file names that are in the specified folder. If there are no files of the specified type, "NO CATALOG" is returned.

**Parameters**

- <char> The type of files to list. Choose from:  
**STATE** - Instrument states (.sta)  
**CORRection** - Calibration Data (.cal)  
**CState** - Instrument state and Calibration data (.cst)  
If unspecified then ALL file types (even unknown types) are listed.
- <folder> String - Any existing folder name. See [Specifying Path Names](#)

**Examples**

```
MMEM:CAT? 'lists all files from the current folder
mmemory:catalog:correction? 'C:\Program Files\Agilent\Network
Analyzer\Documents' 'lists .cal files from the specified folder
```

**Overlapped?** No

**Default** Not applicable

---

**MMEMory:CDIRectory <folder>**

(Read-Write) Changes the folder name.

**Parameters**

- <folder> Any drive and folder name that already exists.  
If the same level as "C:\Program Files\Agilent\Network Analyzer\Documents", then no punctuation is required

```
MMEM:CDIR Service
```

If the new folder is at a different level than "C:\Program Files\Agilent\Network Analyzer\Documents", use a slash (\) before the folder name and enclose in quotes.

```
mmemory:cdirectory '\automation' 'changes default directory up
one level.
```

You can use an absolute path to specify the new folder.

```
mmemory:cdirectory 'c:\automation\service'
```

**Query Syntax** MMEMory:CDIRectory? 'Returns the current folder name

**Return Type** String

**Overlapped?** No

**Default** 'C:\Program Files\Agilent\Network Analyzer\Documents'

---

**MMEMory:COPY <file1>,<file2>**

(Write-only) Copies file1 to file2. Extensions must be specified.

**Parameters**

<file1> String - Name of the file to be copied. See [Specifying Path Names](#)

<file2> String - Name of the file to be created from file1.

**Examples** `MMEM:COPY 'MyFile.cst','YourFile.cst'`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**MMEMemory:DELeTe <file>**

(Write-only) Deletes file. Extensions must be specified.

**Parameters**

<file> String - Name of the file to be deleted. See [Specifying Path Names](#)

**Examples** `MMEM:DEL 'MyFile.cst'`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**MMEMemory:LOAD[:<char>] <file>**

(Write-only) Loads the specified file.

**Parameters**

<char> The type of file to load. Choose from:

**STATE** - Instrument states (.sta)

**CORRection** - Calibration Data (.cal)

**CState** - Instrument state and Calibration data (.cst)

If <char> is unspecified, the extension must be included in the filename.

If an extension is specified in <file> that does not agree with <char> then no action is taken.

<file> String - Name of the file to be loaded. See [Specifying Path Names](#)

**Examples** `MMEM:LOAD 'MyFile.cst'`  
`mmemory:load:state 'MyInstState'`

---

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

### **MMEMory:MDIRectory <folder>**

(Write-only) Makes a folder.

#### **Parameters**

<folder> String - Name of the folder to make. See [Specifying Path Names](#)

**Examples** `MMEM:MDIR 'MyFolder'`  
`mmemory:mdirectory 'c:\NewFolder'`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

### **MMEMory:MOVE <file1>,<file2>**

(Write-only) Renames <file1> to <file2>. File extensions must be specified.

#### **Parameters**

<file1> String - Name of the file to be renamed. See [Specifying Path Names](#)

<file2> String - Name of the new file.

**Examples** `MMEM:MOVE 'MyFile.cst','YourFile.cst'`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

### **MMEMory:RDIRectory <folder>**

(Write-only) Removes the specified folder.

**Parameters**

<folder> String - Name of the folder to remove. See [Specifying Path Names](#)

**Examples** `MMEM:RDIR 'MyFolder'`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**MMEMory:STORE[:<char>] <file>**

(Write-only) Stores the specified file (.sta, .cal, .cst, .s1p, .s2p, and .s3p.).

Learn about [saving SnP files on the PNA](#).

To save \*.cti files, use [MMEM:STOR:CITI:DATA](#) or [MMEM:STOR:CITI:FORM](#).

**Parameters**

<char> The type of file to store. Choose from:  
**STATe** - Instrument states (.sta)  
**CORRection** - Calibration Data (.cal)  
**CSTate** - Instrument state and Calibration data (.cst)  
No <char> is specified for s1p, s2p and s3p  
If unspecified, then the extension must be included in the filename.  
If an extension is specified in <file> that does not agree with <char> then no action is taken.

<file> String - Name of any valid file that is not already in existence. See [Specifying Path Names](#)

**Examples** `MMEM:STOR:STAT 'myState'`  
`mmemory:store 'c:\bin\myState.sta'`  
`MMEM:STOR 'MyData.S2P'`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**MMEMory:STOR:CITI:DATA <filename>**

(Write only) Saves UNFORMATTED trace data to .cti file. [Learn more.](#)

### Parameters

<filename> Any drive and folder name that already exists.  
If the same level as "C:\Program Files\Agilent\Network Analyzer\Documents", then no punctuation is required

```
MMEM:STOR:CITI:DATA MYCITIFile
```

If the new folder is at a different level than "C:\Program Files\Agilent\Network Analyzer\Documents", use a slash (\) before the folder name and enclose in quotes.

```
mmemory:cdirectory '\automation' 'changes default directory up one level.'
```

You can use an absolute path to specify the new folder.

```
mmemory:cdirectory 'c:\automation\service'
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** C:\Program Files\Agilent\Network Analyzer\Documents'

---

## MMEMory:STORe:CITI:FORMat <filename>

(Write only) Saves FORMATTED trace data to .cti file. [Learn more.](#)

### Parameters

<filename> Any drive and folder name that already exists.  
If the same level as "C:\Program Files\Agilent\Network Analyzer\Documents", then no punctuation is required

```
MMEM:STOR:CITI:DATA MYFile
```

If the new folder is at a different level than "C:\Program Files\Agilent\Network Analyzer\Documents", use a slash (\) before the folder name and enclose in quotes.

```
mmemory:cdirectory '\automation' 'changes default directory up one level.'
```

You can use an absolute path to specify the new folder.

```
mmemory:cdirectory 'c:\automation\service'
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** C:\Program Files\Agilent\Network Analyzer\Documents'

---

## MMEMory:STORe:TRACe:CONTents:CITifile <char>

(Read-Write) Specifies the contents of subsequent citifile save statements. (See [Data Define Saves](#))

**Parameters**

- <char> Choose from:
  - SING** - Single trace
  - DISP** - All displayed traces
  - AUTO** - All displayed traces

**Examples** `MMEM:STOR:TRAC:CONT:CIT SING`

**Query Syntax** MMEMory:STORe:TRACe:CONTents?

**Return Type** Character

**Overlapped?** No

**Default** Auto

---

**MMEMory:STORe:TRACe:FORMat:CITifile <char>**

(Read-Write) Specifies the format of subsequent citifile save statements. (See [Data Define Saves](#))

**Parameters**

- <char> Format in which the citifile will be saved with subsequent `MMEMory:STORe:CITi:FORMat` statements. Choose from:
  - MA** - Linear Magnitude / degrees
  - DB** - Log Magnitude / degrees
  - RI** - Real / Imaginary
  - AUTO** - Format in which the trace is already displayed. If other than Log Mag, Linear Magnitude, or Real/Imag, then the format will be in Real/Imag.

**Examples** `MMEM:STOR:TRAC:FORM:CIT MA`

**Query Syntax** MMEMory:STORe:TRACe:FORMat:CITifile?

**Return Type** Character

**Overlapped?** No

**Default** Auto'

---

**MMEMory:STORe:TRACe:FORMat:SNP <char>**

(Read-Write) Specifies the format of subsequent .s1p, .s2p, .s3p save statements. (See [Data Define Saves](#)).

### Parameters

<char> Choose from:

**MA** - Linear Magnitude / degrees

**DB** - Log Magnitude / degrees

**RI** - Real / Imaginary

**AUTO** - data is output in currently selected trace format. If other than LogMag, LinMag, or Real/Imag, then output is in Real/Imag.

**Examples** `MMEM:STOR:TRAC:FORM:SNP MA`

**Query Syntax** `MMEMory:STORe:TRACe:FORMat:SNP?`

**Return Type** Character

**Overlapped?** No

**Default** Auto'

---

### MMEMory:TRANSfer <fileName>,<dataBlock>

(Read-Write) Transfers data between the PNA and an external controller. Other MMEM commands transfer data between the PNA application and the PNA hard drive. If <fileName> already exists, it will be overwritten. The file must be no larger than 20MB.

To read **trace data** from the PNA in block format, use [CALC:DATA](#).

### Parameters

<fileName> String - File name. See [Specifying Path Names](#)

<dataBlock> [Block Data](#) - The contents of the file.

The data block is a block of binary data. Use the following syntax:

`#<num_digits><byte count><data bytes><NL><END>`

where:

`<num_digits>` specifies how many digits are contained in `<byte_count>`

`<byte_count>` specifies how many data bytes will follow in `<data bytes>`

**Example** `See example program`

**Query Syntax** `MMEMory:TRANSfer? <fileName>`

Reads block data from the specified file location.

**Overlapped?** No

**Default** Not applicable





## Output Command

---

[Learn about Power](#)

### **OUTPut[:STATe] <ON | OFF>**

(Read-Write) Turns RF power from the source ON or OFF.

See note about source power state with instrument state save and recall.

#### **Parameters**

<ON | OFF> **ON** (or 1) - turns RF power ON  
**OFF** (or 0) - turns RF power OFF

**Examples** `OUTP ON`  
`output:state off`

**Query Syntax** `OUTPut[:STATe]?`

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

## Route Command

---

[Learn about Frequency Offset](#)

### ROUTe:PATH:LOOP:R1 <char>

(Read-Write) Throws internal switch to reference receiver. This feature is only available on PNA models with [Option 081](#) - external reference switch. See [block diagram of the reference switch](#).

#### Parameters

<char> Position of the switch. Choose from:

**INTernal** - bypass R1 Loop. Connects the port 1 source directly to the R1 receiver.

**EXTernal** - flow through R1 Loop. Allows direct access to the R1 receiver through the Reference 1 front-panel connectors.

#### Examples

```
ROUT:PATH:LOOP:R1 INT
route:path:loop:r1 external
```

**Query Syntax** ROUTe:PATH:LOOP:R1?

**Return Type** Character


**Overlapped?** No

**Default** INTernal

## Sense:Average Commands

---

Sets sweep-to-sweep averaging parameters. Averaging is a noise reduction technique that averages each data point over a user-specified number of sweeps. Averaging affects all of the measurements in the channel.



- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - See an [example](#) using some of these commands.
  - [Learn about Averaging](#)
- 

### SENSe<num>:AVERage:CLEAr

(Write-only) Clears and restarts averaging of the measurement data. Must also set [SENS:AVER:STATe\] ON](#)

#### Parameters

<num> Any existing channel number; if unspecified, value is set to 1.

#### Examples

```
SENS:AVER:CLE
sense2:average:clear
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---



**SENSe<num>:AVERage:COUNT <num>**

(Read-Write) Sets the number of measurement sweeps to combine for an average. Must also set SENS:AVER[:STATe] ON

**Parameters**

- <cnum> Any existing channel number; if unspecified, value is set to 1.
- <num> Number of measurement sweeps to average. Choose any number between: **1** and **1024**

**Examples** `SENS:AVER:COUN 999`  
`sense2:average:count 73`

**Query Syntax** `SENSe<cnum>:AVERAge:COUNT?`

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

**SENSe<cnum>:AVERAge[:STATe] <ON | OFF>**

(Read-Write) Turns trace averaging ON or OFF.

**Parameters**

- <cnum> Any existing channel number; if unspecified, value is set to 1.
- <ON | OFF> **ON** (or 1) - turns averaging ON.  
**OFF** (or 0) - turns averaging OFF.

**Examples** `SENS:AVER ON`  
`sense2:average:state off`

**Query Syntax** `SENSe<cnum>:AVERAge[:STATe]?`

**Return Type** Boolean (1 = ON, 0 = OFF)


**Overlapped?** No

**Default** Off

---

## Sense:Bandwidth Commands

---

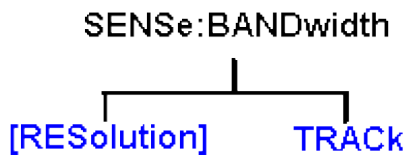

[Learn about IF Bandwidth](#)

[See a list of SCPI commands](#)

---

### SENSe<num>:BANDwidth | BWIDth[:RESolution] <num>

(Read-Write) Sets the bandwidth of the digital IF filter to be used in the measurement. (Use either **Sense:Bandwidth** or **Sense:Bwidth**)

#### Parameters

- <num> Any existing channel number. If unspecified, value is set to 1
- <num> IF Bandwidth in Hz. The list of valid IF Bandwidths is different depending on the PNA model. [\(Click to see the lists.\)](#) If an invalid number is specified, the analyzer will round up to the closest valid number.

#### Examples

```
SENS:BWID 1KHZ
sense2:bandwidth:resolution 1000
```

**Query Syntax** SENSe<num>:BANDwidth | BWIDth[:RESolution]?

**Return Type** Numeric

**Overlapped?** No

**Default** See [Preset IFBW](#) for your PNA model.



---

### SENSe<num>:BANDwidth | BWIDth:TRACk <bool>

(Read-Write) Sets and returns the state of the Reduce IF BW at Low Frequencies feature.  
(Use either **Sense:Bandwidth:Track** or **Sense:Bwidth:Track**).

**Parameters**

<cnm> Any existing channel number. If unspecified, value is set to 1

<bool> Choose from:

**ON** or **1** - Reduce IF BW at Low Frequencies is set ON

**OFF** or **0** - Reduce IF BW at Low Frequencies is set OFF

**Examples**

```
SENS:BWID:TRAC OFF
sense2:bandwidth:track 1
```

**Query Syntax** SENSE<cnm>:BANDwidth | BWIDth:TRACk?

**Return Type** Boolean

**Overlapped?** No


**Default** ON

---

## Sense:Correction Commands

---

Performs and applies measurement calibration and other error correction features.

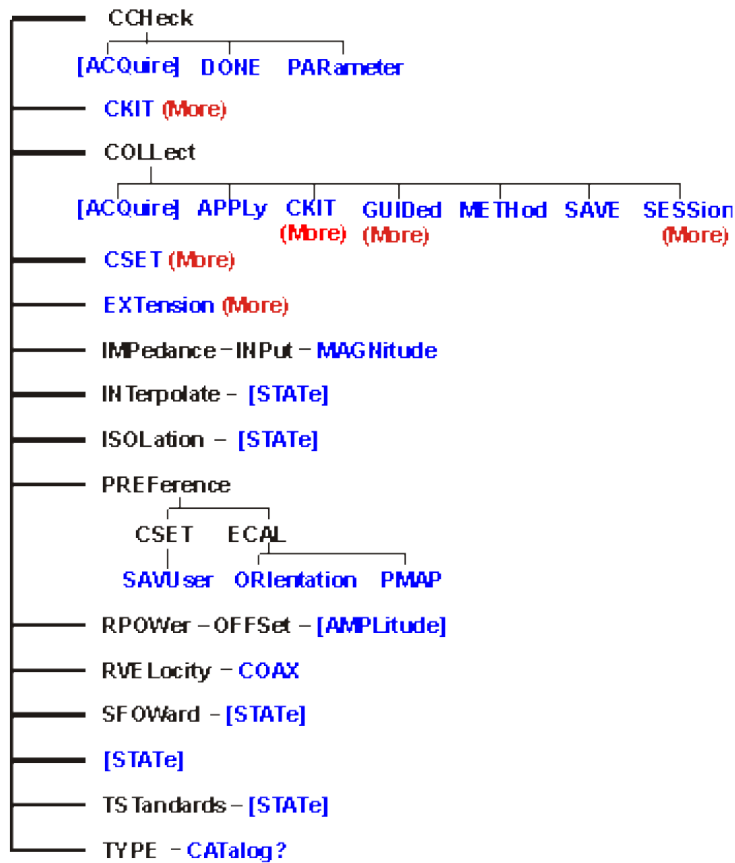

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- New [See Calibrating the PNA Using SCPI](#)
- [See SCPI Example Programs](#)
- [Learn about Measurement Calibration](#)



---

**SENSe<cnum>:CORRection:CCheck[:ACQuire] <mod>[,char]**



(Write-only) Reads the 'confidence data' associated with the specified ECal module and puts it into memory. The measurement is selected using SENS:CORR:CCH:PAR. This command is compatible with \*OPC.

### Parameters

<num> Any existing channel number. If unspecified, value is set to 1.

<mod> ECAL Module that contains the confidence data. Choose from:

**ECAL1**

..through..

**ECAL8**

[char] Optional argument. Specifies which characterization within the ECal module that the confidence data will be read from.

**CHAR0** Factory characterization (data that was stored in the ECal module by Agilent). Default if not specified.

**CHAR1** User characterization #1

**CHAR2** User characterization #2

**CHAR3** User characterization #3

**CHAR4** User characterization #4

**CHAR5** User characterization #5

### Examples

```
SENS:CORR:CCheck ECAL2
```

```
sense2:correction:ccheck:acquire ecal1,char1
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**SENSe<num>:CORRection:CCHeck:DONE**

(Write-only) Concludes the Confidence Check and sets the ECal module back into the idle state.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

**Examples**

```
SENS:CORR:CCH:DONE
sense2:correction:ccheck:done
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

**SENSe<cnum>:CORRection:CCHeck:PARAmeter <Mname>**

(Read-Write) Specifies an existing measurement to be used for the Confidence Check.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<Mname> Name of the measurement you are selecting for the confidence check. The measurement must already exist.

**Examples**

```
SENS:CORR:CCH:PAR 'TEST'
'selects the measurement "test" on channel 1 for the confidence
check

sense2:correction:ccheck:parameter 'test'
'selects the measurement "test" on channel 2 for the confidence
check
```

**Query Syntax** SENSe<cnum>:CORRection:CCHeck:PARAmeter?  
Returns the name of the selected measurement on channel <cnum>.

**Return Type** String

**Overlapped?** No

**Default** Not applicable

---

**SENSe<cnum>:CORRection:COLLect[:ACQuire] <class>[,subclass]**

(Write-only) Measures the specified standards from the selected calibration kit. The calibration kit is selected using the Sense:Correction:Collect:CKIT command.

For using two sets of standards, see SENS:CORR:TST.

**Note:** Before using this command you must select two items:

1. Select a calibration method using SENS:CORR:COLL:METH
2. Select a measurement using CALC:PAR:SEL. You can select one measurement for each channel.

### Parameters

<cnm> Any existing channel number. If unspecified, value is set to 1

<class> **Measures the standards associated with these class labels.** Choose from:

| Label                                   | Forward                                                                                                                                                                                                                  | Reverse |
|-----------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|
| <b>STAN1</b>                            | S11A                                                                                                                                                                                                                     | S22A    |
| <b>STAN2</b>                            | S11B                                                                                                                                                                                                                     | S22B    |
| <b>STAN3</b>                            | S11C                                                                                                                                                                                                                     | S22C    |
| <b>STAN4</b>                            | S21T                                                                                                                                                                                                                     | S12T    |
| <b>STAN5</b>                            | Generic Isolation; not associated with calibration kit definition.                                                                                                                                                       |         |
| <b>ECAL1</b><br>through<br><b>ECAL8</b> | ECAL modules                                                                                                                                                                                                             |         |
| <b>POWer</b>                            | Take a receiver power cal sweep and turn correction ON                                                                                                                                                                   |         |
| <b>SLSET</b>                            | Sets 'sliding load type', and increments the "number of slides" count. The total number of slides is critical to the correct calculation of the sliding load algorithm. See a <a href="#">sliding load cal example</a> . |         |
| <b>SLDONE</b>                           | Computes the sliding load using a circle fit algorithm.                                                                                                                                                                  |         |

[subclass] Optional argument. For mechanical calibration kits, choose from the following to specify the standard to be acquired from the SENS:CORR:COLL:CKIT:ORDER list. If not specified, subclass is set to **SST1**.

- SST1** First standard in the order list
- SST2** Second standard in the order list
- SST3** Third standard in the order list
- SST4** Fourth standard in the order list
- SST5** Fifth standard in the order list
- SST6** Sixth standard in the order list
- SST7** Seventh standard in the order list

If an ECAL module (1 through 8) is specified for <class>, choose one of the following for specifying which characterization within the ECAL module will be used for the acquire. If not specified, the default is **CHAR0**.

- CHAR0** Factory characterization (data that was stored in the ECAL module by Agilent)
- CHAR1** User characterization #1
- CHAR2** User characterization #2
- CHAR3** User characterization #3
- CHAR4** User characterization #4
- CHAR5** User characterization #5

**Examples**

```
SENS:CORR:COLL STAN1

'If SENS:CORR:COLL:CKIT:ORDER2 5,3,7
was specified, the following command measures standard 3 (the
second in the order list)
sense1:correction:collect:acquire stan3,sst2
SENS:CORR:COLL ECAL4
sense2:correction:collect:acquire ecal2,char1
```

- Query Syntax** Not applicable
- Overlapped?** No
- Default** Not applicable

**SENSe<cnum>:CORRection:COLLect:APPLy**

(Write-only) Applies error terms to the measurement that is selected using Calc:Par:Select.

---

**Note:** Before using this command you must select a measurement using CALC:PAR:SEL. You can select one measurement for each channel.

---

**Note:** This command is only necessary if you need to modify error terms. If you do not need to modify error terms, SENSE<cnum>:CORRection:COLLect:SAVE calculates and then automatically applies error terms after you use SENS:CORR:COLL:ACQuire to measure cal standards.

---

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

### Example

```
1. CALCulate2:PARAmeter:SElect S21_2 'select the measurement to
 apply terms to
2. SENSE2:CORRection:COLLect:METHod SPARSOLT 'set type of cal
 method.
3. CALCulate2:DATA? SCORR1 'download the error term of interest
4. 'Modify the error term here
5. CALCulate2:DATA SCORR1 'upload the error term of interest
6. SENSE2:CORRection:COLLect:APPLY 'applies the error terms to
 the measurement
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

---

## SENSe<cnum>:CORRection:COLLect:METHod <char>

(Read-Write) Sets the calibration method (also known as 'Calibration Type' on calibration dialog box.) To set the Cal Type for a Cal Set, use CALC:CORR:TYPE.

---

**Note:** Before using this command you must select a measurement using CALC:PAR:SEL. You can select one measurement for each channel.

---

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<char> Choose from:

| Method                            | Description                          |
|-----------------------------------|--------------------------------------|
| <b>NONE</b>                       | No Cal method                        |
| <b>REFL1OPEN</b>                  | Response Open                        |
| <b>REFL1SHORT</b> or <b>REFL1</b> | Response Short                       |
| <b>REFL3</b>                      | Full 1 port                          |
| <b>RPOWer</b>                     | Receiver Power Cal                   |
| <b>TRAN1</b>                      | Response Thru                        |
| <b>TRAN2</b>                      | Response Thru and Isolation          |
| <b>SPARSOLT</b>                   | Full SOLT 2 port                     |
| <b>SPARTRL</b>                    | TRL Cal (not available on all PNAs.) |

**Examples** `SENS:CORR:COLL:METH REFL1`  
`sense2:correction:collect:method sparsolt`

**Query Syntax** `SENSe<cnun>:CORRection:COLLect:METhod?`

**Return Type** Character

**Overlapped?** No

**Default** Not Applicable

## **SENSe<cnun>:CORRection:COLLect:SAVE**

(Write-only) Calculates the error terms using the selected :METhod and applies the error terms to the selected measurement (turns error correction ON.) Does NOT save the calibration error-terms.

Do NOT use this command during an ECAL.

**Note:** Before using this command you must select a measurement using `CALC:PAR:SEL`. You can select one measurement for each channel.

### **Parameters**

<cnun> Any existing channel number. If unspecified, value is set to 1

**Examples** `SENS:CORR:COLL:SAVE`  
`sense2:correction:collect:save`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not applicable

## **SENSe:CORRection:IMPedance:INPut:MAGNitude <num>**

(Read-Write) Sets and returns the system impedance value for the analyzer.

**Parameters**

<num> System Impedance value in ohms. Choose any number between 0 and 1000 ohms.

**Examples**

```
SENS:CORR:IMP:INP:MAGN 75
sense:correction:impedance:input:magnitude 50.5
```

**Query Syntax** SENSE:CORRection:IMPedance:  
INPUt:MAGNitude?

**Return Type** Numeric

**Overlapped?** No

**Default** 50

---

**SENSe<cnum>:CORRection:INTerpolate[:STATe] <ON | OFF>**

(Read-Write) Turns correction interpolation ON or OFF.

**Note:** Before using this command you must select a measurement using CALC:PAR:SEL. You can select one measurement for each channel.

---

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns interpolation ON.  
**OFF** (or 0) - turns interpolation OFF.

**Examples**

```
SENS:CORR:INT ON
sense2:correction:interpolate:state off
```

**Query Syntax** SENSe<cnum>:CORRection:INTerpolate[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

**SENSe<cnum>:CORRection:ISOLation[:STATe] <ON | OFF> OBSOLETE**

This command no longer works beginning in the PNA 5.2 release. To perform isolation as part of an unguided calibration, you must explicitly measure the isolation standard using [SENS:CORR:COLL:ACQ Stan5](#). See Example program.

(Read-Write) Turns isolation cal ON or OFF during Full 2-port calibration. If this command is not sent, the default state is to **disable** Isolation.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns isolation ON.  
**OFF** (or 0) - turns isolation OFF.

#### Examples

```
SENS:CORR:ISOL ON
sense2:correction:isolation:state off
```

**Query Syntax** SENSE<cnum>:CORRection:ISOLation[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF - (Isolation disabled)

---

### SENSE:CORRection:PREFeRence:CSET:SAVUser <bool>

(Read-Write) Specifies whether the cal data is automatically saved to a User Cal Set file when performing a SCPI calibration. Cal data is always saved to a Cal Register regardless of this setting.

This setting remains until changed by another execution of the command.

Learn about [Cal Registers and User Cal Sets](#).

#### Parameters

<bool> **True** or **1** - Cal is automatically saved to a User Cal Set file when performing a SCPI calibration. The Cal Set name is automatically generated.

**False** or **0** - Cal is NOT automatically saved to a User Cal Set. To save a calibration to a User Cal Set, use [SENS:CORR:COLL:GUID:INIT](#).

#### Examples

```
SENS:CORR:PREF:CSET:SAVU 1
sense:correction:preference:cset:savuser 0
```

**Query Syntax** SENSE:CORRection:PREFeRence:CSET:SAVUser?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF (0)

---

### SENSE:CORRection:PREFeRence:ECAL:ORlentation[:STATe] <ON|OFF>



(Read-Write) Specifies whether or not the PNA should perform orientation of the ECal module during calibration. Orientation is a technique by which the PNA automatically determines which ports of the module are connected to which ports of the PNA. Orientation begins to fail at very low power levels or if there is much attenuation in the path between the PNA and the ECal module. If orientation is turned OFF, the SENS:CORR:PREF:ECAL:PMAP command must be used to specify the port connections before performing a cal.

---

**Note:** For 3-port or 4-port measurements, when orientation is OFF, you are not allowed to specify how the ECAL module is connected. Instead, the PNA determines the orientation. Use SENS:CORR:COLL:GUID:DESC? to query the orientation. The PNA does not verify that you made the connection properly.

---

### Parameters

<bool> ECAL orientation state. Choose from:  
**ON** or **(1)** - PNA performs orientation of the ECal module.  
**OFF** or **(0)** - PNA does NOT performs orientation of the ECal module.

### Examples

```
SENS:CORR:PREF:ECAL:ORI OFF
sense:correction:preference:ecal:orientation:state on
```

**Query Syntax** SENSE:CORRection:PREFErence:ECAL:ORlentation[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON (1)

---

## SENSe:CORRection:PREFErence:ECAL:PMAP <module>,<string>

(Read-Write) When ECal module orientation is turned OFF (SENS:CORR:PREF:ECAL:ORI), this command specifies the port mapping (which ports of the module are connected to which ports of the PNA) prior to performing ECal calibrations.

### Parameters

<module> Specifies which ECal module this port map is being applied to. Choose from:  
**ECAL1**  
.through.  
**ECAL8**

<string> Format this parameter in the following manner:

Aw,Bx,Cy,Dz

where

- A, B, C, and D are literal ports on the ECAL module
- w,x,y, and z are substituted for PNA port numbers to which the ECAL module port is connected.

Ports of the module which are not used are omitted from the string.

For example, on a 4-port ECal module with

port A connected to PNA port 2

port B connected to PNA port 3

port C not connected

port D connected to PNA port 1

the string would be: A2,B3,D1

If either the receive port or source port (or load port for 2-port cal) of the CALC:PAR:SElECTed measurement is not in this string and orientation is OFF, an attempt to perform an ECal calibration will fail.

**Examples**

```
SENS:CORR:PREF:ECAL:PMAP ECAL2, 'A1,B2'
sense:correction:preference:ecal:pmap ecal3, 'a2,b1,c3'
```

**Query Syntax** SENSE:CORRection:PREFeRence:ECAL:PMAP? <module>

**Return Type** String

**Overlapped?** No

**Default** Null string ()

## SENSe<cnum>:CORRection:RPOWER:OFFSet[:AMPLitude] <num>

(Read-Write) Adjusts a receiver power cal to account for components or adapters that are added between the source port and receiver while performing this cal. For more information, see [Receiver Cal](#).

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<num> Offset Value in dB. Specify loss as a negative number; and gain as a positive number. Choose a number between -200 and 200.

**Examples**

```
SENS:CORR:RPOW:OFFS .5
sense2:correction:rpower:offset:amplitude .-5
```

**Query Syntax** SENSe<cnum>:CORRection:RPOWER:OFFSet[:AMPLitude]?

**Return Type** Numeric

**Overlapped?** No

Default 0

---

### SENSe<cnum>:CORRection:RVELocity:COAX <num>

(Read-Write) Sets the velocity factor to be used with Electrical Delay and Port Extensions.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<num> Velocity factor. Choose a number between **0** and **10**  
(.66 polyethylene dielectric; .7 teflon dielectric)

#### Examples

```
SENS:CORR:RVEL:COAX .66
sense2:correction:rvelocity:coax .70
```

**Query Syntax** SENSe<cnum>:CORRection:RVELocity:COAX?

**Return Type** Numeric

**Overlapped?** No

Default 1

---

### SENSe:CORRection:SFORward[:STATe] <boolean>

(Read-Write) Sets the direction a calibration will be performed when only one set of standards is used.

Use SENSe:CORRection:TSTandards[:STATe] **OFF** to specify that only one set of standards will be used.

#### Parameters

<boolean> **ON (1)** - FORWARD direction of a 2-port calibration will be performed  
**OFF (0)** - REVERSE direction of a 2-port calibration will be performed

#### Examples

```
SENS:CORR:SFOR 1
sense:correction:sforward:state 0
See an example using this command
```

**Query Syntax** SENSe:CORRection:SFORward[:STATe]?

**Return Type** Boolean

**Overlapped?** No

Default ON

---

### SENSe<cnum>:CORRection[:STATe] <ON | OFF>

(Read-Write) Turns error correction ON and OFF for the specified channel.

**Note:** Before using this command you must select a measurement using CALC:PAR:SEL. You can select one measurement for each channel.

#### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <ON | OFF> **ON** (or 1) - correction is applied to the channel.  
**OFF** (or 0) - correction is NOT applied to the channel.

#### Examples

```
SENS:CORR ON
sense2:correction:state off
```

#### Query Syntax

SENSe<cnum>:CORRection[:STATe]?

To query the error correction state for a measurement, use CALC:CORR:STATe?

#### Return Type

Boolean (1 = ON, 0 = OFF)

#### Overlapped?

No

#### Default

OFF

---

### SENSe:CORRection:TSTandards[:STATe] <boolean>

(Read-Write) Specifies the acquisition of calibration data using TWO set of standards or ONE.

#### Parameters

<boolean> **ON (1)** - TWO sets of standards will be used for full 2-port calibration for both Forward and Reverse parameters.

**OFF (2)** - ONE set of standards will be used for full 2-port calibration.

Set SENSe:CORRection:COLLect:SFORward[:STATe] to **ON** for the forward acquisitions and **OFF** for the reverse acquisitions.

When specifying ON (two sets), the SENS:CORR:COLL:ACQuire command uses the same standard index for each calibration class. To specify the calibration standard gender for each port, you must first ensure that the order of calibration class accurately reflects the configuration of your DUT. For example, for a DUT with a male connector on port 1 and a female connector on port 2, order the devices within the S11 classes (A, B, and C) such that the MALE standards are first in the list. Then order the S22 classes specifying the FEMALE standards as the first in the list.

#### Examples

```
SENS:CORR:TST 1
sense:correction:tstandard:state 0
See an example using this command
```

#### Query Syntax

SENSe:CORRection:TSTandards[:STATe]?

#### Return Type

Boolean

**Overlapped?** No

**Default** ON

---

## **SENSe:CORRection:TYPE:CATalog? <char>**

(Read-Write) Lists the Cal Types in the PNA by either GUID or registered name. **Critical Note:**

### **Parameters**

<char> Specifies the type of list. Choose from:  
**GUID** - the registered GUID of the Cal Type  
**NAME** - the registered name of the Cal Type

**Examples** `SENS:CORR:TYPE:CAT? GUID`

**Query Syntax** `SENSe<num>:CORRection:TYPE:CATalog? <char>`

**Return Type** Comma-separated string


**Overlapped?** No

**Default** Not Applicable

---

## Sense:Correction:Collect:Guided Commands

Performs and applies a GUIDED measurement calibration and other error correction features.

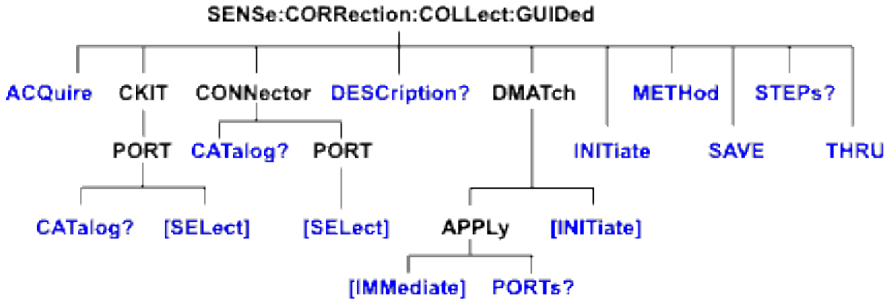

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- See an [example](#) using some of these commands.
- New [See Calibrating the PNA Using SCPI](#)
- [Learn about Measurement Calibration](#)

### SENSe:CORRection:COLLect:GUIDed:ACQuire <std>

(Write-only) Initiates the measurement of the specified calibration standard. Executing this command with an unnecessary standard has no affect.

The measured data is stored and used for subsequent calculations of error correction coefficients. All standards must be measured before a calibration can be completed. Any measurement can be repeated until the [SENSe:CORR:COLL:GUID:SAVE](#) command is executed.

Query the user prompt description using [SENSe:CORR:COLL:GUID:DESC?](#)

Query the required calibration steps using [SENSe:CORR:COLL:GUID:STEP?](#)

#### Parameters



<num> Any existing channel number. If unspecified, value is set to 1

<std> Choose from:STAN1, STAN2, STAN3, through STAN40

#### Examples

```
SENSe:CORR:COLL:GUID:ACQ STAN1
sense:correction:collect:guided:acquire stan1
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

### SENSe:CORRection:COLLect:GUIDed:CKIT:PORT<pnum>:CATalog?

(Read-only) Returns a comma-separated list of valid kits for each port. In addition to mechanical calibration kits, this will include applicable characterizations found within ECal modules currently connected to the PNA. Use items in the list to select the kit to be used with the SENS:CORR:COLL:GUID:CKIT:PORT command.

**Parameters**

<pnum> Any existing port number. If unspecified, value is set to 1

**Examples**

```
SENS:CORR:COLL:GUID:CKIT:PORT1:CAT?
'When "Type N (50) male" is specified for connector type,
returns:
"85054D, 85032F"
```

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:GUIDed:CKIT:PORT<pnum>[:SElect] <kit>**

(Read-Write) Specifies the calibration kit for each port to be used during a guided calibration. An unused port does NOT need to have a specified Cal Kit.

**Note:** Sliding loads are not fully supported from Sens:Corr:Coll:Guided... The **Measure** button must be manually pressed.

---

1. Specify the connector type for the port with SENS:CORR:COLL:GUID:CONN:PORT.
2. Query the valid available kits for the connector on each port with SENS:CORR:COLL:GUID:CKIT:PORT:CAT?
3. Specify the kit using this command.
4. Perform a query of this command. If the <kit> parameter was incorrectly entered, an error will be returned.

**Parameters**

<pnum> Any existing port number. If unspecified, value is set to 1

<kit> Calibration kit to be used for the specified port.

**Examples**

```
SENS:CORR:COLL:GUID:CKIT:PORT1 '85055A'

sense:correction:collect:ckit:port2:select '85092-60010 User 1
ECal'
```

**Query Syntax** SENSe:CORRection:COLLect:GUIDed:CKIT:PORT<pnum>[:SElect]?

**Return Type** String - If the <kit> parameter was incorrectly entered while writing, an error will be returned.

**Overlapped?** No

**Default** Not Applicable

---

## **SENSe:CORRection:COLLect:GUIDed:CONNector:CATalog?**

(Read only) Returns a list of valid connectors based on the connector descriptions of the available cal kits. Use an item from the returned list to specify a connector for SENS:CORR:COLL:GUID:CONN:PORT

**Examples** `SENS:CORR:COLL:GUID:CONN:CAT?`

Returns:

```
Type N (50) female, Type N (50) male, APC 7 (50), 3.5 mm (50)
male, 3.5 mm (50) female, User Connector A
```

**Return Type** Comma separated string values

**Overlapped?** No

**Default** Not Applicable

---

## **SENSe:CORRection:COLLect:GUIDed:CONNector:PORT<pnum>[:SElect] <conn>**

(Read-Write) Specifies a connector type for every port during the Guided Calibration procedure. Valid connector names are stored within calibration kits. Some cal kits may include both male and female connectors. Therefore, specifying connector gender may be required.

Unused ports must be defined as or Not used. If all ports are defined as "Not used", a guided calibration cannot be performed.

- A single port with a valid <conn> name indicates a 1-Port calibration will be performed.
- Two ports with valid <conn> names indicate either a 2-Port or TRL calibration will be performed depending on the standards definition found within the cal kit and the capability of the analyzer. (The analyzer must have 4 receivers for TRL calibrations.).
- Three ports with valid <conn> names indicate a 3-Port calibration will be performed.
- Four ports with valid <conn> names indicate a 4-Port calibration will be performed.

---

### **Note:**

1. Use SENS:CORR:COLL:GUID:CONN:CAT? to query available connectors before specifying the port connector.
  2. Select a connector type using this command.
  3. Perform a query of this command. If the <conn> parameter was incorrectly entered, an error will be returned.
  4. Specify the cal kit to use for each port with SENS:CORR:COLL:GUID:CKIT:PORT
- 

### **Parameters**

<pnum> Any existing port number. If unspecified, value is set to 1



<conn> DUT connector type to connect with analyzer port <pnum>

Some kits may include both male and female connectors so specifying gender may be required.

Valid connector names are stored within calibration kits. Query available connectors using SENSe:CORRection:COLLect:GUIDed:CONNector:CATalog?

**Examples**

```
SENS:CORR:COLL:GUID:CONN:PORT1 'Type N (50) female'
'Indicates the DUT port that connects with the analyzer's Port1
is a TypeN 50 ohm Female connector.'
```

**Query Syntax** SENSE:CORRection:COLLect:GUIDed:CONNector:PORT<pnum>[:SElect]?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

### SENSe:CORRection:COLLect:GUIDed:DESCription? <step>

(Read-only) Returns the connection description for the specified calibration step.

**Parameters**

<step> A number from 1 to the number of steps required to complete the calibration (Use SENS:CORR:COLL:GUID:STEP? to query the number of steps )

**Examples**

```
SENS:CORR:COLL:GUID:DESC? 10
'Returns:
Connect APC 7 Open to port3'
```

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

### SENSe:CORRection:COLLect:GUIDed:DMATch:APPLY[:IMMEDIATE] [<CalSetGUID>]

(Write-only) Specifies a Cal Set as a source of delta match correction.

If 'CalSetGUID' is not specified, then the Global Delta Match Cal Set is assumed. An error is returned if the **specified** Cal Set does not meet the following Delta Match criteria. The Global Delta Match Cal can ALWAYS be applied.

- Must have been performed using ECal or as a guided mechanical cal (not Unguided).
- Must have the same start freq, stop freq, and number of points as the channel being calibrated.
- Must calibrate the ports that are required by the TRL or Unknown Thru cal as indicated by SENS:CORR:COLL:GUID:DMATch:APPLY:PORTs?.

[Learn more about Delta match calibration.](#)

See example of a complete [Delta Match calibration.](#)

#### Parameters

<CalSetGUID> Optional. GUID of the Cal Set to use. If unspecified, the Global Delta Match Cal Set is used.

#### Examples

```
SENS:CORR:COLL:GUID:DMAT:APPL
sense:correction:collect:guided:dmatch:apply:immediate
"{2B893E7A-971A-11d5-8D6C-00108334AE96}"
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe:CORRection:COLLection:GUIDed:DMATch:APPLY:PORTs?

(Read-only) Returns the port numbers for which delta match correction is required. 0 (zero) is returned if the Cal does NOT require Delta Match correction for one of the following reasons:

- The Cal does NOT involve Unknown THRU or TRL. You specify this using SENS:CORR:COLL:GUID:METH <UNKN | TRL>.
- The cal DOES involve Unknown THRU or TRL, but the delta match data can be calculated by the Unknown Thru or TRL Cal. [Learn how this is possible.](#) However, you can force the Cal to use the Delta Match data from a Cal Set.

[Learn more about Delta match calibration.](#)

See example of a complete [Delta Match calibration.](#)

#### Parameters

#### Examples

```
SENS:CORR:COLL:GUID:APPLY:PORT?
```

```
'Returns:
```

```
1,2,3
```

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

## **SENSe:CORRection:COLLect:GUIDed:DMATch[:INITiate] <conn>,<cKit>**

(Write-only) Initiates a global delta match calibration.

[Learn more about Global Delta Match calibration.](#)

See example of a complete [Delta Match calibration.](#)

### **Parameters**

<conn> **String**. Connector type for port 1. All other ports are set automatically.

<cKit> **String** Cal Kit for all ports. If incorrectly entered while writing, an error is returned.

### **Examples**

```
SENS:CORR:COLL:GUID:DMAT "APC 3.5 female","85052B"
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## **SENSe<cnum>:CORRection:COLLect:GUIDed:INITiate [GUID [,bool]]**

(Write-only) Initiates a guided calibration. Either create a new cal set or optionally add to / overwrite a specified cal set.

The PNA determines the measurements needed to perform the calibration using the settings specified from the [SENS:CORR:COLL:GUID:CONN:PORT](#) and [SENS:CORR:COLL:GUID:CKIT:PORT](#) commands.

After this command is executed, subsequent commands can be used to query the number of measurement steps, issue the acquisition commands, query the connection description strings, and subsequently complete a guided calibration.

### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<GUID> Optional argument. If not specified a new calset is created.

Calset GUID in the form: "{GUID}"; including quotes and curly brackets.

The guided cal that is being initiated either supplements the existing cal set, or overwrites the cal set depending on the method, connectors, and ports selected. [Learn more about Cal Sets.](#)

Must be a valid GUID; an error is reported if the GUID is not found.

Query all Cal Set GUIDs with [SENS:CORR:CSET:CAT?](#)

<bool> Optional argument.

**False (0)** If cal set stimulus settings differ from the existing channel, do not change channel stimulus settings. Return an error. This is the default setting if not specified.

**True (1)** If cal set stimulus settings differ from the existing channel, change the channel stimulus settings to match the cal set settings..

**Examples** `SENS:CORR:COLL:GUID:INIT "{2B893E7A-971A-11d5-8D6C-00108334AE96}",1`  
`sense2:correction:collect:guided:initiate`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## SENSe:CORRection:COLLect:GUIDed:METHod <char>

(Read-Write) Selects from one of several algorithms available for performing the THRU portion of a guided calibration. [Learn more about THRU methods.](#)

### Parameters

<char> **DEFAULT** - Informs guided calibrations to use the default algorithm when computing the number of needed standards acquisition steps. (default selection if omitted.)

**ADAP** - Use the adapter removal algorithm

**FLUSH** - Use with insertable devices.

**UNKN** - Use the Unknown THRU algorithm for 2-Port calibrations for non-insertable devices.

**DEFined** - Use the THRU definition that you stored in the cal kit file, or ECal module.

**TRL** - Select TRL Cal Type for guided cals. Valid for "TRL ready" Cal Kits with properly assigned TRL cal classes.

**SOLT** - Select SOLT Cal Type for 2-Port guided cals. Valid for any kit with properly assigned SOLT cal classes.

**Examples** `SENS:CORR:COLL:GUID:METH ADAP`  
`sense:correction:collect:guided:method unkn`

**Query Syntax** SENSe:CORRection:COLLect:GUIDed:METHod?

**Return Type** Character

**Overlapped?** No

**Default** DEFAULT

---

## SENSe:CORRection:COLLect:GUIDed:SAVE

(Write-only) Completes the guided cal by computing the error correction terms, turning Correction ON, and saving the calibration to a Cal Set.

If all of the required standards have not been measured, the calibration will not complete properly.

**Examples** `SENS:CORR:COLL:GUID:SAVE`  
`sense2:correction:collect:guided:save`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe:CORRection:COLLect:GUIDed:STEPs?

(Read-only) Returns the number of measurement steps required to complete the current guided calibration. This command is sent after the `SENS:CORR:COLL:GUID:INIT`, `SENS:CORR:COLL:GUID:CONN:PORT` and `SENS:CORR:COLL:GUID:CKIT:PORT` commands.

**Examples** `SENS:CORR:COLL:GUID:STEP?`  
`sense2:correction:collect:guided:steps?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

### SENSe:CORRection:COLLect:GUIDed:THRU:PORTs <t1a, t1b, t2a, t2b, t3a, t3b>

(Read-Write) For 3-port and 4-port calibrations ONLY. Specifies the port pairs for the thru connections of the calibration.

#### Parameters

- <t1a,...> Specify Port numbers in pairs:
- For 3-port cals, specify two pairs.
  - For 4-port cals, specify three pairs.

t1a, t1b (Thru1 - port A and port B)

t2a, t2b (Thru2 - port A and port B)

t3a, t3b (Thru3 - port A and port B)

**Examples** `SENS:CORR:COLL:GUID:THRU:PORT 1,2,1,3,1,4 '4-port measurement`  
`sense:correction:collect:guided:thru:ports 1,2,2,3 '3-port`  
`measurement`

**Query Syntax** `SENSe:CORRection:COLLect:GUIDed:THRU:PORTs?`

**Return Type** Numeric

**Overlapped?** No


**Default** Port pairings that were used in the previous cal.

---

## Sense:Correction:Ckit Commands

---

Manages the list of cal kits that are installed in the PNA.

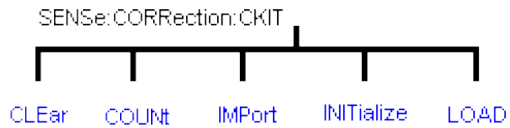

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Modifying Cal Kits](#)
  - New [See Calibrating the PNA Using SCPI](#)
- 

### SENSe<num>:CORRection:CKIT:CLEAr[:IMMediate]

(Write-only) Deletes ALL installed cal kits.

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

**Examples** SENS:CORR:CKIT:CLE

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe<num>:CORRection:CKIT:COUNT?

(Read-only) Returns the number of installed cal kits.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

**Examples** `SENS:CORR:CKIT:COUNT?`

**Query Syntax** `SENS:CORR:CKIT:COUNT?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<cnum>:CORRection:CKIT:IMPoRT <string>**

(Write-only) Imports the specified cal kit (.ckt file) and appends the imported kit to the end of the list of kits whenever the file import succeeds.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1.

<string> Path and cal kit name.

**Examples** `SENSe2:CORRection:CKIT:IMPoRT "C:\Program Files\Agilent\Network Analyzer\Documents\85033D.ckt"`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<cnum>:CORRection:CKIT:INITialize[:IMMediate]**



(Write-only) Restores all default factory installed cal kits.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

**Examples**

```
SENS:CORR:CKIT:INITialize
sense2:correction:ckit:initialize
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<cnum>:CORRection:CKIT:LOAD <string>**

(Write-only) Loads the specified collection of cal kits from a .wks file. You can make your own collection of cal kits from the Advanced Modify Cal Kit menu.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<string> Path and file name of the cal kit collection.

**Examples**

```
sense2:correction:ckit:load "C:\Program Files\Agilent\Network
Analyzer\PnaCalKits\factory\MyCalKits.wks
```

**Query Syntax** Not Applicable


**Overlapped?** No

**Default** Not Applicable

## Sense:Correction:Collect:Ckit Commands

---

Use to change the definitions of calibration kit standards.

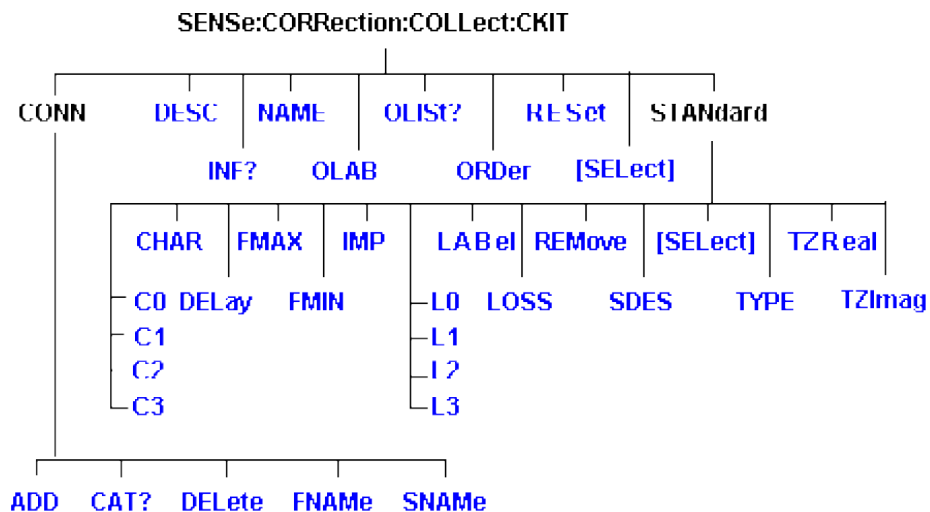


Click on a blue keyword to view the command details.

Most of these commands act on the currently selected standard from the currently selected calibration kit.

- To select a Calibration kit, use [SENSe:CORRection:COLLect:CKIT:SEL](#).
- To select a Calibration standard, use [SENSe:CORRection:COLLect:CKIT:STAN:SEL](#)
- See a [List](#) of all commands in this block.
- See an **example** program that [CREATES a New Cal Kit](#)
- See an **example** program that [MODIFIES an Existing Cal Kit](#)
- [Learn about Modifying Cal Kits](#)

---

**Note:** You should provide data for every definition field - for every standard in your calibration kit. If a field is not , the default value may not be what you expect.

---

**SENSe:CORRection:COLLect:CKIT:CONNector:ADD**  
<family>,<start>,<stop>,<z0>,<gender>,<media>,<cutoff>

(Write only) Creates a new connector. The connector is automatically added to the list of available connectors for the currently selected cal kit. If a connector includes both male and female connectors, each connector must be added separately.

### Parameters

- <family> (String) Name of connector family. Limited to 50 characters.
- <start> Start frequency
- <stop> Stop frequency
- <z0> Characteristic Impedance of the connector in ohms.
- <gender> Connector gender. Choose from:  
MALE  
FEMALE  
NONE
- <media> Media of the connector. Choose from:  
**COAX** - coaxial  
**WAVE** - waveguide
- <cutoff> Cutoff frequency of the connector (waveguide only).

### Examples

```
SENS:CORR:COLL:CKIT:CONN:ADD "PSC 1.8 mm",0 HZ,999.9
GHZ,50,FEMALE,COAX,0.0
SENS:CORR:COLL:CKIT:CONN:ADD "PSC 1.8 mm",0 HZ,999.9
GHZ,50,MALE,COAX,0.0
```

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:CONNector:CATalog?**

(Read-only) Returns a comma-separated list of all connectors defined within the currently selected cal kit. The returned string includes the connector family name followed by the connector gender, if any. Kits may include a primary connector family name and additional connector family names.

Connector family names are case sensitive. A connector family named "PSC 2.4" is different from a connector family named "psc 2.4".

Learn more about [Connector Family Name](#)

**Parameters** None

**Examples**

```
SENS:CORR:COLL:CKIT:CONN:CAT?
'Returned string
"Type-N (50) male, Type-N (50) female"
```

**Overlapped?** No

**Default** Not Applicable

---

### **SENSe:CORRection:COLLect:CKIT:CONNector:DELeTe**

(Write-only) Deletes the primary connector family name from the selected kit. The PNA allows multiple connector families for each kit. If a kit includes multiple connector families, only the first listed (primary) connector family name is deleted.

Once the connector family is deleted, the connector may not be assigned to any new or existing standard within the kit.

The previously defined standards retain their association to the deleted connector name. To reassign standards to a new connector family name, use [SENS:CORR:COLL:CKIT:CONN:SNAME](#).

**Parameters** None

**Examples**

```
SENS:CORR:COLL:CKIT:CONN:DEL
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### **SENSe:CORRection:COLLect:CKIT:CONNector:FNAME <name>**

(Read-Write) Replaces the primary connector family name from the selected kit with a new connector family name. The connector family name is replaced in all standards in the kit that share that name. The PNA allows multiple connector families for each kit. If a kit includes multiple connector families, only the first listed (primary) connector family name is replaced. Use the query form of this command to return the name of the primary connector family.

#### Parameters

<name> New connector family name. Limited to 50 characters.

#### Examples

```
SENS:CORR:COLL:CKIT:CONN:FNAME 'MYPSC35'
```

```
Sense:correction:collect:ckit:connector:name 'My Type N'
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:CONNector:FNAME?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

### SENSe:CORRection:COLLect:CKIT:CONNector:SNAME <family>,<gender>,<port>

(Read-Write) Assigns a family name to the currently selected standard from the currently selected kit. Specify each port of a 2-port standard individually. Use the query form of this command to read the connector family name assigned to the current standard. The name is not assigned unless the connector family name is previously defined within the selected kit.

#### Parameters

<family> String. Connector family name.

<gender> Connector gender. Choose from:  
MALE  
FEMALE  
NONE

<port> Number of the connector port to be assigned the connector family name. 2-port standards such as a thru line must be assigned separately. It is not relevant which connector is port 1 or port 2.

**1** Specifies a 1-port standard or the first port of a 2-port standard.

**2** Specifies the second port of a 2-port standard.

#### Examples

```
SENS:CORR:COLL:CKIT:CONN:SNAME "Type-N (50)",MALE,1
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:CONNector:SNAME?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

## SENSe:CORRection:COLLect:CKIT:DESCRiption <string>

(Read-Write) Modifies the cal kit description field of the selected kit. This description appears in the [Edit PNA Cal Kit dialog box](#).

### Parameters

<string> Description of the cal kit. Limited to 50 characters.

**Examples** `SENS:CORR:COLL:CKIT:DESC "My New CalKit"`

**Query Syntax** `SENSe:CORRection:COLLect:CKIT:DESCRiption?`

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

## SENSe:CORRection:COLLect:CKIT:INFormation? <module>[,char]

(Read Only) Reads characterization information from an ECal module. This command returns the same string as the [GetECALModuleInfo](#) method on the [Calibrator](#) COM object.

### Parameters

<module> Specifies which ECal module to read from. Choose from:

**ECAL1**

.through.

**ECAL8**

[char] Optional argument.

Specifies which characterization within the ECal module to read information from. If this argument is not used, the default is **CHAR0**. **CHAR1** through **CHAR5** are for user characterizations that may have been written to the module by the User Characterization feature on the PNA. Choose from:

**CHAR0** Factory characterization (data that was stored in the ECal module by Agilent)

**CHAR1** User characterization #1

**CHAR2** User characterization #2

**CHAR3** User characterization #3

**CHAR4** User characterization #4

**CHAR5** User characterization #5

**Examples** `SENS:CORR:COLL:CKIT:INF? ECAL4`  
`sense:correction:collect:ckit:information? ecal2,char1`

Example return string:

```
ModelNumber: 85092-60007, SerialNumber: 01386, ConnectorType:
N5FN5F, PortAConnector: Type N (50) female, PortBConnector: Type
N (50) female, MinFreq: 30000, MaxFreq: 9100000000,
NumberOfPoints: 250, Calibrated: July 4 2002
```

**Return Type** Character

**Overlapped?** No

**Default** Not Applicable

---

## **SENSe:CORRection:COLLect:CKIT:NAME <name>**

(Read-Write) Sets a name for the selected calibration kit.

### **Parameters**

<name> Calibration Kit name. Any string name, can include numerics, period, and spaces; any length (although the dialog box display is limited to about 30 characters).

### **Examples**

```
SENSe:CORR:COLL:CKIT:NAME 'MYAPC35'
sense:correction:collect:ckit:name 'mytypen'
```

**Query Syntax** SENSe:CORRection:COLLect:CKIT:NAME?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

## **SENSe:CORRection:COLLect:CKIT:OLABel<class> <name>**

(Read-Write) Sets the label for the calibration class designated by <class>. The label is used in the prompts for connecting the calibration standards associated with that <class>.

### **Parameters**

<class> Number of the calibration class. Choose a number between: 1 and 18. The <class> numbers are associated with the following calibration Classes:

|   | <b>Class</b> | <b>Description</b>  |
|---|--------------|---------------------|
| 1 | S11A         | Reflection standard |
| 2 | S11B         | Reflection standard |
| 3 | S11C         | Reflection standard |
| 4 | S21T         | Thru/Delay standard |
| 5 | S22A         | Reflection standard |
| 6 | S22B         | Reflection standard |
| 7 | S22C         | Reflection standard |
| 8 | S12T         | Thru/Delay standard |

### 3-port analyzers only

|    |      |                     |
|----|------|---------------------|
| 9  | S33A | Reflection standard |
| 10 | S33B | Reflection standard |
| 11 | S33C | Reflection standard |
| 12 | S32T | Thru/Delay standard |
| 13 | S23T | Thru/Delay standard |
| 14 | S31T | Thru/Delay standard |
| 15 | S13T | Thru/Delay standard |

### TRL Calibrations

|    |         |                  |
|----|---------|------------------|
| 16 | TRL "T" | Thru standard    |
| 17 | TRL "R" | Reflect standard |
| 18 | TRL "L" | Line standard    |

<name> Label for the calibration class. Must be enclosed in quotes. Any string between 1 and 12 characters long. Cannot begin with a numeric.

#### Examples

```
SENS:CORR:COLL:CKIT:OLAB3 'LOADS'
sense:correction:collect:ckit:olabel14 'Thru'
```

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

**SENSe:CORRection:COLLect:CKIT:OLIST[class]?**



(Read-only) Returns seven values of standards that are assigned to the specified class.

**Parameters**

<class> Number of the calibration class to be queried. The <class> numbers are associated with the following calibration Classes:

|   | <b>Class</b> | <b>Description</b>  |
|---|--------------|---------------------|
| 1 | S11A         | Reflection standard |
| 2 | S11B         | Reflection standard |
| 3 | S11C         | Reflection standard |
| 4 | S21T         | Thru/Delay standard |
| 5 | S22A         | Reflection standard |
| 6 | S22B         | Reflection standard |
| 7 | S22C         | Reflection standard |
| 8 | S12T         | Thru/Delay standard |

**3-port analyzers ONLY**

**4-port analyzers use S11 and S22 classes (see example program)**

|    |      |                     |
|----|------|---------------------|
| 9  | S33A | Reflection standard |
| 10 | S33B | Reflection standard |
| 11 | S33C | Reflection standard |
| 12 | S32T | Thru/Delay standard |
| 13 | S23T | Thru/Delay standard |
| 14 | S31T | Thru/Delay standard |
| 15 | S13T | Thru/Delay standard |

**TRL Calibrations**

|    |         |                  |
|----|---------|------------------|
| 16 | TRL "T" | Thru standard    |
| 17 | TRL "R" | Reflect standard |
| 18 | TRL "L" | Thru standard    |

**Examples**

**SENS:CORR:COLL:CKIT:OLIST8?**  
Always returns 7 standard numbers. Unassigned standards return 0

**Return Type** Numeric; returns the <class> number of the selected standard.

**Overlapped?** No

**Default** Not Applicable

**SENSe:CORRection:COLLect:CKIT:ORDer<class> <std> [,<std>] [,<std>] [,<std>] [,<std>] [,<std>]**

(Read-Write) Sets a standard number to a calibration class. Does **NOT** set or dictate the order for measuring the standards. For more information, see Assigning Standards to a Calibration Class

**Parameters**

<class> Number of the calibration class that is assigned to <standard>. Choose a number between: **1** and **18**. The <class> numbers are associated with the following calibration Classes:

|   | <b>Class</b> | <b>Description</b>  |
|---|--------------|---------------------|
| 1 | S11A         | Reflection standard |
| 2 | S11B         | Reflection standard |
| 3 | S11C         | Reflection standard |
| 4 | S21T         | Thru/Delay standard |
| 5 | S22A         | Reflection standard |
| 6 | S22B         | Reflection standard |
| 7 | S22C         | Reflection standard |
| 8 | S12T         | Thru/Delay standard |

**3-port analyzers ONLY**

**4-port analyzers use S11 and S22 classes (see example program)**

|    |      |                     |
|----|------|---------------------|
| 9  | S33A | Reflection standard |
| 10 | S33B | Reflection standard |
| 11 | S33C | Reflection standard |
| 12 | S32T | Thru/Delay standard |
| 13 | S23T | Thru/Delay standard |
| 14 | S31T | Thru/Delay standard |
| 15 | S13T | Thru/Delay standard |

**TRL Calibration**

|    |         |                  |
|----|---------|------------------|
| 16 | TRL "T" | Thru standard    |
| 17 | TRL "R" | Reflect standard |
| 18 | TRL "L" | Line standard    |

<std> Standard number to be assigned to the class; Choose a standard between 1 and 8. One standard is mandatory; up to six additional standards are optional.

**Examples** Assigns standard 3 to S11A class:  
`SENS:CORR:COLL:CKIT:ORD1 3`  
Assigns standard 2 and 5 to S21T class class:  
`sense:correction:collect:ckit:order4 2,5`

**Query Syntax** SENSE:CORRection:COLLEct:CKIT:ORDeR<class>?  
'Returns only the first standard assigned to the specified class. To query the remaining standards, use SENSE:CORRection:COLLEct:CKIT:OLIST[1-15]?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

### **SENSe:CORRection:COLLEct:CKIT:RESet <num>**

(Write-only) Obsolete in Rev 3.2. Instead use Sens:Corr:Ckit:Init.

Resets the selected calibration kit to factory default definition values.

#### **Parameters**

<num> The number of the calibration kit to be reset. Choose any integer between: 1 and 8

**Examples** `SENS:CORR:COLL:CKIT:RESet 1`  
`sense:correction:collect:ckit:reset 4`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### **SENSe:CORRection:COLLEct:CKIT[:SElect] <num>**

(Read-Write) Selects (makes active) a calibration kit for **performing** a calibration or for **modifying** standards. All subsequent "CKIT" commands that are sent apply to this selected calibration kit. Select a calibration standard using SENSe:CORR:COLL:CKIT:STAN <num>

**Parameters**

<num> The number of the calibration kit. Choose from:  
Use SENSe:CORRection:COLLect:CKIT:RESet to restore Cal Kits to default values.

**Name**

- 1 User Defined 1
- 2 User Defined 2
- 3 User Defined 3
- "
- "
- 48 User Defined 48
- 49 User Defined 49
- 50 User Defined 50
- 99 ECAL module

**Examples**

```
SENSe:CORR:COLL:CKIT 2
sense2:correction:collect:ckit:select 7
```

**Query Syntax** SENSe:CORRection:COLLect:CKIT?

**Return Type** Numeric

**Overlapped?** No

**Default** Last kit selected

---

**SENSe:CORRection:COLLect:CKIT:STANdard:C0 <num>**

(Read-Write) Sets the C0 value (the first capacitance value) for the selected standard.

**Parameters**

<num> Value for C0 in picofarads

**Examples**

The following commands set C0=15 picofarads:

```
SENS:CORR:COLL:CKIT:STAN:C0 15
sense:correction:collect:ckit:standard:c0 15
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:C0?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:C1 <num>**

(Read-Write) Sets the C1 value (the second capacitance value) for the selected standard.

**Parameters**

<num> Value for C1 in picofarads

**Examples**

The following two commands set C1=15 picofarads:

```
SENS:CORR:COLL:CKIT:STAN:C1 15
sense:correction:collect:ckit:standard:c1 15
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:C1?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:C2 <num>**

(Read-Write) Sets the C2 value (the third capacitance value) for the selected standard.

**Parameters**

<num> Value for C2 in picofarads

**Examples**

The following two commands set C2=(-15) picofarads:

```
SENS:CORR:COLL:CKIT:STAN:C2 -15
sense:correction:collect:ckit:standard:c2 -15
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:C2?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:C3 <num>**

(Read-Write) Sets the C3 value (the fourth capacitance value) for the selected standard.

**Parameters**

<num> Value for C3 in picofarads

**Examples**

The following two commands set C3=15 picofarads:

```
SENS:CORR:COLL:CKIT:STAN:C3 15
sense:correction:collect:ckit:standard:c3 15
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:C3?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:CHARacter <char>**

(Read-Write) Sets the media type of the selected calibration standard.

**Parameters**

<char> Media type of the standard. Choose from:  
**Coax** - Coaxial Cable  
**Wave** - Waveguide

**Examples** `SENS:CORR:COLL:CKIT:STAN:CHAR COAX`  
`sense:correction:collect:ckit:standard:character wave`

**Query Syntax** `SENSe:CORRection:COLLect:CKIT:STANdard:CHARacter?`

**Return Type** Numeric

**Overlapped?** No

**Default** Coax

---

**SENSe:CORRection:COLLect:CKIT:STANdard:DELay <num>**

(Read-Write) Sets the electrical delay value for the selected standard.

**Parameters**

<num> Electrical delay in seconds

---

**Examples** `SENS:CORR:COLL:CKIT:STAN:DEL 50e-12`  
`sense2:correction:collect:ckit:standard:delay 50ps`

**Query Syntax** `SENSe:CORRection:COLLect:CKIT:STANdard:DELay?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:FMAX <num>**

(Read-Write) Sets the maximum frequency for the selected standard.

**Parameters**

<num> Maximum frequency in Hertz.

**Examples** `SENS:CORR:COLL:CKIT:STAN:FMAX 9e9`  
`sense:correction:collect:ckit:standard:fmax 9Ghz`

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:FMAX?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:FMIN <num>**

(Read-Write) Sets the minimum frequency for the selected standard.

**Parameters**

<num> Minimum frequency in Hertz.

**Examples** `SENS:CORR:COLL:CKIT:STAN:FMIN 1e3`  
`sense:correction:collect:ckit:standard:fmin 1khz`

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:FMIN?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:IMPedance <num>**



(Read-Write) Sets the characteristic impedance for the selected standard.

**Parameters**

<num> Impedance in Ohms

**Examples**

```
SENS:CORR:COLL:CKIT:STAN:IMP 75
sense:correction:collect:ckit:standard:impedance 50.3
```

**Query Syntax**

SENSe:CORRection:COLLect:CKIT:STANdard:IMPedance?

**Return Type**

Numeric

**Overlapped?**

No

**Default**

50

---

**SENSe:CORRection:COLLect:CKIT:STANdard:L0 <num>**

(Read-Write) Sets the L0 value (the first inductance value) for the selected standard.

**Parameters**

<num> Value for L0 in picohenries

**Examples**

The following two commands set L0=15 picohenries:  

```
SENS:CORR:COLL:CKIT:STAN:L0 15
sense:correction:collect:ckit:standard:l0 15
```

**Query Syntax**

SENSe:CORRection:COLLect:CKIT:STANdard:L0?

**Return Type**

Numeric

**Overlapped?**

No

**Default**

Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:L1 <num>**

(Read-Write) Sets the L1 value (the second inductance value) for the selected standard.

**Parameters**

<num> Value for L1 in picohenries

**Examples**

The following two commands set L1=15 picohenries:

```
SENS:CORR:COLL:CKIT:STAN:L1 15
sense:correction:collect:ckit:standard:l1 15
```

**Query Syntax**

SENSe:CORRection:COLLect:CKIT:STANdard:L1?

**Return Type**

Numeric

**Overlapped?**

No

**Default**

Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:L2 <num>**

(Read-Write) Sets the L2 value (the third inductance value) for the selected standard.

**Parameters**

<num> Value for L2 in picohenries

**Examples**

The following two commands set L2=15 picohenries:

```
SENS:CORR:COLL:CKIT:STAN:L2 15
sense:correction:collect:ckit:standard:l2 15
```

**Query Syntax**

SENSe:CORRection:COLLect:CKIT:STANdard:L2?

**Return Type**

Numeric

**Overlapped?**

No

**Default**

Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:L3 <num>**

(Read-Write) Sets the L3 value (the fourth inductance value) for the selected standard.

**Parameters**

<num> Value for L3 in picohenries

**Examples**

The following two commands set L3=15 picohenries:

```
SENS:CORR:COLL:CKIT:STAN:L3 15
sense:correction:collect:ckit:standard:l3 15
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:L3?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:LABel <name>**

(Read-Write) Sets the label for the selected standard. The label is used to prompt the user to connect the specified standard.

**Parameters**

<name> Label for the standard; Must be enclosed in quotes. Any string between **1** and **12** characters long. Cannot begin with a numeric.

**Examples**

```
SENS:CORR:COLL:CKIT:STAN:LAB 'OPEN'
sense:correction:collect:ckit:standard:label 'Short2'
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:LABel?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:LOSS <num>**

(Read-Write) Sets the insertion loss for the selected standard.

**Parameters**

<num> Insertion loss in Mohms / sec. (MegaOhms per second of electrical delay)

**Examples** `SENS:CORR:COLL:CKIT:STAN:LOSS 3.5e9`  
`sense:correction:collect:ckit:standard:loss 3`

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:LOSS?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:REMOve**

(Write only) Deletes the selected standard from the selected cal kit.

**Examples** `SENS:CORR:COLL:CKIT:STAN:REMOve`

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:SDEScRiption <string>**

(Read-Write) Modifies the description of the selected standard of the selected kit. This description appears in the [edit kit dialog box](#).

**Parameters**

<string> Description of the standard.

**Examples** `SENS:CORR:COLL:CKIT:STAN:SDES "My New Standard"`

**Query Syntax** SENSE:CORRection:COLLect:STANdard:SDEScRiption?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard[:SELEct] <num>**

(Read-Write) Selects the calibration standard. All subsequent "CKIT" commands to modify a standard will apply to the selected standard. Select a calibration kit using SENS:CORR:COLL:CKIT:SEL

**Parameters**

<num> Number of the standard. Choose any number between:  
**1 and 30**

**Examples**

```
SENS:CORR:COLL:CKIT:STAN 3
sense:correction:collect:ckit:standard:select 8
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard[:SElect]?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

**SENSe:CORRection:COLLect:CKIT:STANdard:TYPE <char>**

(Read-Write) Sets the type for the selected standard.

**Parameters**

<char> Choose from:  
**OPEN**  
**SHORT**  
**LOAD**  
**SLOAD** (sliding load)  
**THRU** (through)  
**ARBI**(arbitrary)

**Examples**

```
SENS:CORR:COLL:CKIT:STAN:TYPE LOAD
sense:correction:collect:ckit:standard:type short
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:TYPE?

**Return Type** Character

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:TZReal <num>**

(Read-Write) Sets the TZReal component value of the Terminal Impedance for the selected standard.

**Note:** Only applicable when the Standard Type is set to **ARBI**

---

**Parameters**

<num> Value for TZReal in Ohms

---

**Examples**

The following commands set TZReal=15 Ohms:

```
SENS:CORR:COLL:CKIT:STAN:TZReal 15
sense:correction:collect:ckit:standard:TZReal 15
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:TZReal?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe:CORRection:COLLect:CKIT:STANdard:TZImag <num>**

(Read-Write) Sets the TZImag component value of the Terminal Impedance for the selected standard.

**Note:** Only applicable when the Standard Type is set to **ARBI**

---

**Parameters**

<num> Value for TZImag in Ohms

**Examples**

The following two commands set TZImag=15 Ohms:

```
SENS:CORR:COLL:CKIT:STAN:TZImag 15
sense:correction:collect:ckit:standard:TZImag 15
```

**Query Syntax** SENSE:CORRection:COLLect:CKIT:STANdard:TZImag?

**Return Type** Numeric

**Overlapped?** No


**Default** Not Applicable

---

## Sense:Correction:Cset Commands

---

Performs actions on calibration sets.

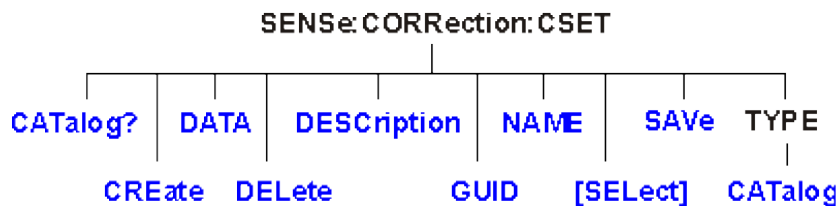

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Cal Sets](#)
- New [See Calibrating the PNA Using SCPI](#)

---

### SENSE:CORRection:CSET:CATalog?

(Read-only) Returns a string containing a list of comma-separated GUIDs for Cal Sets in the following format:

```
{FD6F863E-9719-11d5-8D6C-00108334AE96},
{1B03B2CE-971A-11d5-8D6C-00108334AE96}
```

#### Parameters

#### Examples

```
SENS:CORR:CSET:CAT?
sense2:correction:cset:catalog?
```

**Overlapped?** No

**Default** Not Applicable



---

### SENSE<num>:CORRection:CSET:CREate <name>

(Write-only) Creates an empty Cal Set and attaches it to the specified channel.

**Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<name> Name of the Cal Set. Spaces or punctuation NOT allowed.

**Examples** `SENS:CORR:CSET:CRE 'My2Port'`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<num>:CORRection:CSET:DATA <eterm, portA, portB,> <block>**

(Read-Write) Read or Write a specific error term from/to the Cal Set currently attached to the specified channel.

**Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<eterm, portA, portB> **Error Term, Port pair of the specified error term.**

Although not all error terms use two port numbers, two are required by the PNA in all cases. Each port number must be between 1 and the maximum number of ports on the PNA.:

**EDIR** - directivity

portA: the port at which directivity is measured

portB: ignored (but still subject to the above limit check).

**ESRM** - source match

portA: the port at which source match is measured

portB: ignored (but still subject to the above limit check).

**ERFT** - reflection tracking

portA: the port at which reflection tracking is measured

portB: ignored (but still subject to the above limit check).



**ELDM** - load match

portA: the port at which load match is measured

portB: the drive port.

Load match is measured with a cable connected between the measured port (portA) and the drive port (portB).

The cal system requires that the complete matrix of loadmatch arrays be filled. In most cases you can measure loadmatch once at a port, driven by any other port. Then use that data for all variations of the receive port. (The exception is the 3-port PNA models, which requires the loadmatch-measured port to be driven by every other port.)

For example: Measure the loadmatch at port2 while driving port1. Then upload this same data to the following arrays:

ELDM,2,1,<data>

ELDM,2,3,<data>

ELDM,2,4,<data>

**ETRT**: transmission tracking

portA: the receive port

portB: the source port for this measurement

**EXTLK** - crosstalk

portA: the receive port

portB: the source port for this measurement

A full 4-port calibration requires the following terms be uploaded:

|                       |   | PORT B                            |                                   |                                   |                                   |
|-----------------------|---|-----------------------------------|-----------------------------------|-----------------------------------|-----------------------------------|
|                       |   | 1                                 | 2                                 | 3                                 | 4                                 |
| P<br>O<br>R<br>T<br>A | 1 | EDIR,1,1<br>ERFT,1,1<br>ESRM,1,1  | ELDM,1,2<br>ETRT,1,2<br>EXTLK,1,2 | ELDM,1,3<br>ETRT,1,3<br>EXTLK,1,3 | ELDM,1,4<br>ETRT,1,4<br>EXTLK,1,4 |
|                       | 2 | ELDM,2,1<br>ETRT,2,1<br>EXTLK,2,1 | EDIR,2,2<br>ERFT,2,2<br>ESRM,2,2  | ELDM,2,3<br>ETRT,2,3<br>EXTLK,2,3 | ELDM,2,4<br>ETRT,2,4<br>EXTLK,2,4 |
|                       | 3 | ELDM,3,1<br>ETRT,3,1<br>EXTLK,3,1 | ELDM,3,2<br>ETRT,3,2<br>EXTLK,3,2 | EDIR,3,3<br>ERFT,3,3<br>ESRM,3,3  | ELDM,3,4<br>ETRT,3,4<br>EXTLK,3,4 |
|                       | 4 | ELDM,4,1<br>ETRT,4,1<br>EXTLK,4,1 | ELDM,4,2<br>ETRT,4,2<br>EXTLK,4,2 | ELDM,4,3<br>ETRT,4,3<br>EXTLK,4,3 | EDIR,4,4<br>ERFT,4,4<br>ESRM,4,4  |

Reflection terms

Transmission terms

**Examples** `SENS:CORR:CSET:DATA EXTLK,3,1`

**Query Syntax** `SENSe<num>:CORRection:CSET:DATA? <eterm,portA, portB>`

**Return Type** Block data

**Overlapped?** No

**Default** Not Applicable

---

### **SENSe<num>:CORRection:CSET:DELeTe <string>**

(Write-only) Deletes a Cal Set from the set of available Cal Sets. This command immediately updates the Cal Set file on the hard drive. Using the Cal Sets collection is a convenient way to manage Cal Sets.

#### **Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<string> The GUID of the Cal Set to be deleted. The curly brackets and hyphens must be included. Not case sensitive.

**Examples** `SENS:CORR:CSET:DEL '{2B893E7A-971A-11d5-8D6C-00108334AE96}'  
sense2:correction:cset:delete '{2B893E7A-971A-11d5-8D6C-  
00108334AE96}'`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### **SENSe<num>:CORRection:CSET:DESCRiption <string>**

(Read-Write) Sets or returns the descriptive string assigned to the selected Cal Set. Change this string so that you can easily identify each Cal Set. Select the Cal Set using SENSe:CORRection:CSET:GUID

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <string> The descriptive string associated with the currently-selected Cal Set

**Examples** `SENS:CORR:CSET:DESC 'MyCalSet'`  
`sense2:correction:cset:description 'thisCalSet'`

**Query Syntax** SENSE<num>:CORRection:CSET:DESCription?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<num>:CORRection:CSET:GUID <string>**

(Read-Write) Selects the Cal Set identified by the string parameter (GUID) and applies it to the specified channel. A Cal Set cannot be selected for a channel which is not ON.

If the stimulus settings of the selected Cal Set differ from those of the selected channel, the instrument will automatically change the channel's settings to match the Cal Set.

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <string> GUID of the desired Cal Set. The curly brackets and hyphens must be included.

**Examples** `SENS:CORR:CSET:GUID '{2B893E7A-971A-11d5-8D6C-00108334AE96}'`  
`sense2:correction:cset:guid '{2B893E7A-971A-11d5-8D6C-00108334AE96}'`

**Query Syntax** SENSE<num>:CORRection:CSET:GUID?  
Returns the GUID of the currently-selected Cal Set for the specified channel.

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<num>:CORRection:CSET:NAME <string>**

(Read-Write) Sets or queries the name of the Cal Set currently attached to the specified channel.

**Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <string> Name of the Cal Set. Spaces or punctuation NOT allowed.

**Examples**

```
SENS:CORR:CSET:NAME 'MyCalSet'
sense2:correction:cset:name 'thisCalSet'
```

**Query Syntax** SENSE<cnum>:CORRection:CSET:NAME?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<cnum>:CORRection:CSET[:SElect] <char>**

(Read-Write) Restores a state from memory. The file name is "**CSETx.cst**" where x is the user number assigned to <char>, and .cst specifies a cal set and instrument state. This is not the same syntax as a file saved through the default choices from the front panel, which is "**at00x.cst**". For more information on the file naming syntax, see the [MMEMemory](#) subsystem. Learn more about [Instrument/Cal States](#).

To save a state to memory, use [SENS:CORR:CSET:SAVE](#).

**Note:** This command does NOT select a Cal Set for a channel. To select a Cal Set, use [SENS:CORR:CSET:GUID](#).

---

**Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <char> Choose from:
  - DEF** - Presets the analyzer
  - USER01** - Restores User01 calibration data
  - USER02** - Restores User02 calibration data through...
  - USER10** - Restores User10 calibration data

**Examples**

```
SENS:CORR:CSET DEF
sense2:correction:cset:select user02
```

**Query Syntax** SENSe<cnum>:CORRection:CSET[:SElect]?

**Return Type** Character

**Overlapped?** No

**Default** DEF

---

## SENSe<cnum>:CORRection:CSET:SAVE <char>

(Read Write) Write a correction data set to memory or read the last correction set saved. The file name is saved as "CSETx.cst" where x is the user number assigned to <char>, and .cst specifies a cal set and instrument state. This is not the same syntax as a file saved through the default choices from the front panel, which is "at00x.cst". For more information on the file naming syntax, see the [MMEMory](#) subsystem. Learn more about [Instrument/Cal States](#).

This command also saves the channel's Cal Set to the PNA hard drive. For example, use this command after writing data to a Cal Set using [SENS:CORR:CSET:DATA](#)

To recall a state from memory, use [SENS:CORR:CSET](#).

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <char> Choose from:  
USER01  
USER02...  
USER10

### Examples

```
SENS:CORR:CSET:SAVE USER03
sense2:correction:cset:save user09
```

**Query Syntax** SENSe<cnum>:CORRection:CSET:SAVE?  
Queries the last correction set saved.

**Return Type** Character

**Overlapped?** No

**Default** Not applicable

---

## SENSe<ch>:CORRection:CSET:TYPE:CATalog? [format]

(Read-only) Query the Cal Types available in the selected Cal Set. You can specify the output format: a comma separated list of Guids or a list of names.

Note: CalTypes in earlier versions of PNA (pre 3.0) were indicated by a pre defined enumeration. In 3.0 the identity of the CalType has been expanded to support runtime detectable contribution calibration types. CalTypes are now identified by GUID's (128 bit number) and a name (string).

---

### Parameters

- <ch> Any existing channel number. If unspecified, value is set to 1
- [format] (Optional) Format of the output of cal types. choose from:  
**NAME** - (default) returns a list of cal type string names.  
**GUID** - returns a list of cal type GUIDs

### Examples

```
SENS:CORR:CSET:TYPE:CAT? NAME
SENS2:CORRection:CSET:TYPE:CAT?
```

---

**Return Type** string


**Overlapped?** No

**Default** Not Applicable

## Sense:Correction:Extension Commands

---

Performs and applies Port Extensions.

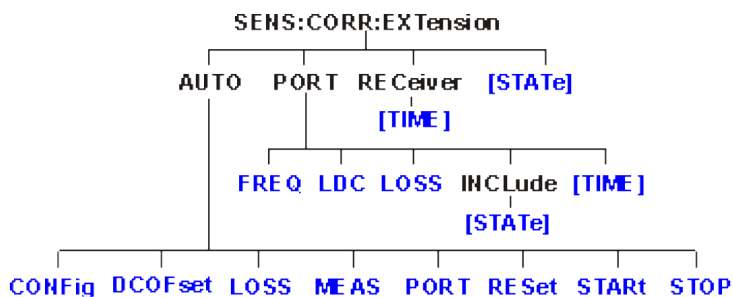

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Port Extensions](#)
- 

### SENSe<num>:CORRection:EXTension:AUTO:CONFig <char>

(Read-Write) Sets the frequencies used to calculate Automatic Port Extension. [Learn more about calculating Automatic Port Extension.](#)

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<char> Frequencies to be used:

**CSPN** Use current frequency span.

**AMKR** - Use active marker frequency.

**USPN** - Use custom user span. Use [SENS:CORR:EXT:AUTO:STAR](#) and [SENS:CORR:EXT:AUTO:STOP](#) to specify start and stop frequency.



#### Examples

```
SENS:CORR:EXT:AUTO:CONF CSPN
sense2:correction:extension:auto:config amkr
```

**Query Syntax** SENSe<num>:CORRection:EXTension:AUTO:CONFig ?

**Return Type** Character

**Overlapped?** No

**Default** CSPN

---

### SENSe<num>:CORRection:EXTension:AUTO:DCOFset <bool>

(Read-Write) Specifies whether or not to include DC Offset as part of automatic port extension. [Learn more about Automatic DC Offset](#). Only allowed when [SENS:CORR:EXT:AUTO:LOSS](#) is set to ON.

#### Parameters

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <bool> ON (or 1) - Includes DC Offset correction.  
OFF (or 0) - Does NOT include DC Offset correction.

**Examples** `SENS:CORR:EXT:AUTO:DCOF 1`  
`sense2:correction:extension:auto:dcoffset off`

**Query Syntax** SENSE<cnm>:CORRection:EXTension:AUTO:DCOFFset?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF (0)

---

### SENSE<cnm>:CORRection:EXTension:AUTO:LOSS <bool>

(Read-Write) Specifies whether or not to include loss correction as part of automatic port extension. [Learn more about Loss Compensation](#) in port extension.

#### Parameters

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <bool> ON (or 1) - Includes Loss correction.  
OFF (or 0) - Does NOT include Loss correction.

**Examples** `SENS:CORR:EXT:AUTO:LOSS 1`  
`sense2:correction:extension:auto:loss off`

**Query Syntax** SENSE<cnm>:CORRection:EXTension:AUTO:LOSS?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF (0)

---

### SENSE<cnm>:CORRection:EXTension:AUTO:MEASure <char>



(Write-only) Measures either an OPEN or SHORT standard. When this command is sent, the PNA acquires the measurement with which to set automatic port extensions. [Learn more about which standard to measure.](#)

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<char> Standard to be measured. Choose from:

**OPEN** Measure OPEN standard

**SHORT** Measure SHORT standard

#### Examples

```
SENS:CORR:EXT:AUTO:MEAS OPEN
sense2:correction:extension:auto:measure short
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe<cnum>:CORRection:EXTension:AUTO:PORT<n> <bool>

(Read-Write) Enables and disables automatic port extensions on the specified port.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<n> PNA Port number to enable or disable for automatic port extensions.

<bool> ON (or 1) - Enable

OFF (or 0) - Disable

#### Examples

```
SENS:CORR:EXT:AUTO:PORT2 0
sense2:correction:extension:auto:port4 on
```

**Query Syntax** SENSe<cnum>:CORRection:EXTension:AUTO:PORT<n>?

**Return Type** Boolean

**Overlapped?** No

**Default** All ports ON (enabled)

---

### SENSe<cnum>:CORRection:EXTension:AUTO:RESet

(Write-only) Clears old port extension delay and loss data in preparation for acquiring new data. Send this command prior to sending a new series of `SENS:CORR:EXT:AUTO:MEAS`. If acquiring both OPEN and SHORT standards, do not send this command between those acquisitions.

**Parameters**

<cnun> Any existing channel number. If unspecified, value is set to 1

**Examples**

```
SENS:CORR:EXT:AUTO:RES
sense2:correction:extension:auto:reset
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<cnun>:CORRection:EXTension:AUTO:STARt <value>**

(Read-Write) Set the start frequency for custom user span. [Learn more about User Span.](#)

**Parameters**

<cnun> Any existing channel number. If unspecified, value is set to 1

<value> User span start value. Must be within the frequency range of the active channel and less than the value set by `SENS:CORR:EXT:AUTO:STOP`.

**Examples**

```
SENS:CORR:EXT:AUTO:STAR 1E9
sense2:correction:extension:auto:start 200e6
```

**Query Syntax** `SENSe<cnun>:CORRection:EXTension:AUTO:STARt <value>?`

**Return Type** Numeric

**Overlapped?** No

**Default** Start frequency of the current active channel.

---

**SENSe<cnun>:CORRection:EXTension:AUTO:STOP <value>**

(Read-Write) Set the stop frequency for custom user span. [Learn more about User span.](#)

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <value> User span stop value. Must be within the frequency range of the active channel and greater than the value set by SENS:CORR:EXT:AUTO:START

**Examples**

```
SENS:CORR:EXT:AUTO:STOP 1E9
sense2:correction:extension:auto:stop 200e6
```

**Query Syntax** SENSE<num>:CORRection:EXTension:AUTO:STOP <value>?

**Return Type** Numeric

**Overlapped?** No

**Default** Stop frequency of the current active channel.

---

**SENSe<num>:CORRection:EXTension:PORT<pnum>:FREQ<n> <value>**

(Read-Write) Sets and returns the frequency "Use" number (1|2) for the specified port number.

[Learn about Loss Compensation values.](#)

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <pnum> Port Number that will receive the freq/loss settings. If unspecified, value is set to 1.
- <n> Frequency "Use" number. Choose from 1 or 2. If unspecified, value is set to 1.
- <value> Frequency value. Choose a frequency within the frequency span of the PNA.

**Examples**

```
SENS:CORR:EXT:PORT1:FREQ1 10E9
sense2:correction:extension:port2:freq2:2E10
```

**Query Syntax** SENSE<num>:CORRection:EXTension:PORT<pnum>:FREQ<n>?

**Return Type** Numeric

**Overlapped?** No

**Default** 1 GHz

---

**SENSe<num>:CORRection:EXTension:PORT<pnum>:INCLude<n>:STATe <bool>**

(Read-Write) Sets and returns the ON/OFF state for the use of the Loss and Freq values for the specified port number.

[Learn about Loss compensation values.](#)

---

**Note:** This command affects ALL measurements on the specified channel.

---

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <pnum> Port Number that will receive the Freq/Loss settings. If unspecified, value is set to 1.
- <n> Freq and Loss pair. Choose from 1 or 2. If unspecified, value is set to 1.
- <value> State of Freq and Loss values for port extension.  
**0 or OFF** Specified Freq and Loss values are OFF  
**1 or ON** Specified Freq and Loss values are ON

### Examples

```
SENS:CORR:EXT:PORT:INCL 0
sense2:correction:extension:port2:include:state on
```

**Query Syntax** SENSE<cnum>:CORRection:EXTension:PORT<pnum>:INCLude:STATe?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF

---

## SENSe<cnum>:CORRection:EXTension:PORT<pnum>:LDC <value>

(Read-Write) Sets and returns the Port Loss at DC value for the specified port number.

[Learn about Loss compensation values.](#)

---

**Note:** This command affects ALL measurements on the specified channel.

---

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <pnum> Port number to receive Loss value. If unspecified, value is set to 1.
- <value> Loss in dB. Choose a value between -90 and 90

### Examples

```
SENS:CORR:EXT:PORT:LDC 1.5
sense2:correction:extension:port2:ldc .1
```

**Query Syntax** SENSE<cnum>:CORRection:EXTension:PORT<pnum>:LDC?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## **SENSe<cnum>:CORRection:EXTension:PORT<pnum>:LOSS<n> <value>**

(Read-Write) Sets and returns the Loss value for the specified port number.

[Learn about Loss compensation values.](#)

---

**Note:** This command affects ALL measurements on the specified channel.

---

### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<pnum> Port Number that will receive the Freq/Loss settings. If unspecified, value is set to 1.

<n> Loss "Use" number. Choose from 1 or 2. If unspecified, value is set to 1.

<value> Loss in dB. Choose a value between -90 and 90

### **Examples**

```
SENS:CORR:EXT:PORT:LOSS1 1
sense2:correction:extension:port2:loss2 .1
```

**Query Syntax** SENSe<cnum>:CORRection:EXTension:PORT<pnum>:LOSS<n>?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## **SENSe<cnum>:CORRection:EXTension:PORT<pnum>[:TIME] <num>**

(Read-Write) Sets the extension value at the specified port. Must also set SENS:CORR:EXT ON.

**Note:** This command affects ALL measurements on the specified channel.

---

**Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <pnum> Port Number that will receive the extension. If unspecified, value is set to 1.
- <num> The port extension in seconds; may include suffix. Choose a number between: -1E18 and 1E18

**Examples**

```
SENS:CORR:EXT:PORT 2MS
sense2:correction:extension:port2 .00025
```

**Query Syntax** SENSE<cnum>:CORRection:EXTension:PORT<pnum> [:TIME]?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**SENSe<cnum>:CORRection:EXTension:RECEiver<Rnum>[:TIME] <num> OBSOLETE**

(Read-Write) This command has NO replacement and no longer works.

Sets the extension value at the specified receiver. Must also set SENS:CORR:EXT ON.

**Note:** Before using this command you must select a measurement using CALC:PAR:SEL. You can select one measurement for each channel.

---

**Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <Rnum> Number of the receiver that will receive the extension. If unspecified, value is set to 1  
Choose from:
  - 1 for Receiver A
  - 2 for Receiver B
- <num> The electrical length in seconds; may include suffix. Choose a number between: -10 and 10

**Examples**

```
SENS:CORR:EXT:REC 2MS
sense2:correction:extension:receiver2:time .00025
```

**Query Syntax** SENSe<cnum>:CORRection:EXTension:RECEiver<Rnum> [:TIME]?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**SENSe<cnum>:CORRection:EXTension[:STATe] <ON | OFF>**

(Read-Write) Turns port extensions ON or OFF.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns port extensions ON.  
**OFF** (or 0) - turns port extensions is OFF.

**Examples**

```
SENS:CORR:EXT ON
sense2:correction:extension:state off
```

**Query Syntax** SENSe<cnum>:CORRection:EXTension[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---


## Sense:Correction:Collect:Session Commands

---

The commands in this topic are common to perform both SMC and VMC calibrations. A calibration session is simply a term used to describe an instance of a custom (SMC or VMC) calibration. For more commands, see [SESS:SMC](#) and [SESS:VMC](#).

Commands to read ([STEP?](#)) and describe ([DESC?](#)) each step are provided to facilitate a remote user interface.

To perform a **NON** - SMC or VMC calibration, use either [Guided](#) or [Mechanical](#) SCPI commands.

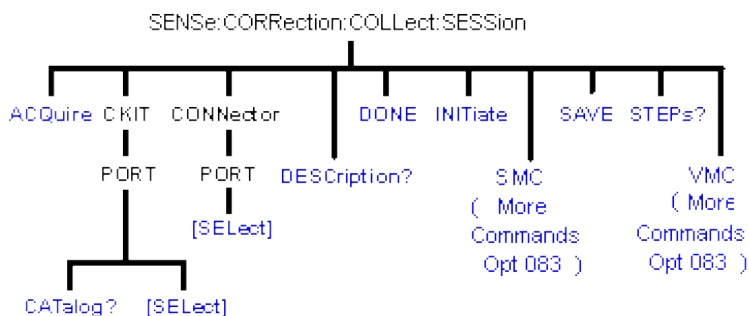

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - See a SCPI [SMC](#) and [VMC](#) calibration.
  - Learn about [SMC](#) and [VMC](#) calibrations
- 

### SENSe<ch>:CORRection:COLLect:SESSion<n>:ACQuire <step>

(Write only) Acquire a calibration measurement.

#### Parameters

<ch> Any existing channel number. If unspecified, value is set to 1.

<n> Session number. Choose from 1 to 16.

<step> Step number to acquire. Use [SENSe:CORRection:COLLect:SESSion:STEPS?](#) to find the number of steps required for the calibration.

#### Examples

```
SENSe2:CORR:COLL:SESS6:ACQ 5
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe<ch>:CORRection:COLLect:SESSion<n>:CKIT:PORT<p>:CATalog?



(Read only) Returns a list of cal kits that are compatible with the connector on port <p>. The port connector type is set with SENS:CORR:COLL:SESS:CONN:PORT

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> Session number. Choose from 1 to 16.
- <p> Port number of connector to query for compatible cal kits.

**Examples** `SENS2:CORR:COLL:SESS6:CKIT:PORT2:CAT?`

**Return Type** Comma separated string values

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:CORRection:COLLect:SESSion<n>:CKIT:PORT<p>[:SELection] <calkit>**

(Read-Write) Set or return the Cal Kit for the specified port. Use SENS:CORR:COLL:SESS:CKIT:PORT:CAT? to list compatible Cal Kits.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16.
- <p> Port number for which to set cal kit.
- <calkit> Cal Kit Name

**Examples** `SENS:CORR:COLL:SESS:CKIT:PORT:SEL 85091A`  
`SENS2:CORR:COLL:SESS6:CKIT:PORT2:SEL?`

**Query Syntax** `SENS<ch>:CORR:COLL:SESS<n>:CKIT:PORT<p>[:SEL] ?`

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:CORRection:COLLect:SESSion<n>:CONN:PORT<p>[:SEL] <conn>**

(Read-Write) Set the connector type and sex for the specified port number. Catalog valid connector types using SENS:CORR:COLL:GUID:CONN:CAT?

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16.
- <p> Port number for which to select a connector type.
- <conn> Name of the connector type

**Examples** `SENS2:CORR:COLL:SESS6:CONN:PORT1:SEL "N Type"`

**Query Syntax** `SENS<ch>:CORR:COLL:SESS<n>:CONN:PORT<p>[:SEL]?`

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:CORRection:COLLEct:SESSion<n>:DESC? <step>**

(Read-only) Returns the connection prompt for the step. List the number of steps in the calibration using SENS:CORR:COLL:SESS:STEPS?.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16.
- <step> Step number

**Examples** `SENS1:CORR:COLL:SESS6:DESC?3`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:CORRection:COLLEct:SESSion<n>:DONE**

(Write only) Ends the calibration sessions. Use SAVE? to calculate error terms and save the CalSet.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

**Examples** `SENS1:CORR:COLL:SESS6:DONE`

**Query Syntax** Not Applicable

Overlapped? No

Default Not Applicable

---

**SENSe<ch>:CORRection:COLLect:SESSion<n>:INITiate <string>**

(Write only) Initiates an SMC or VMC calibration session. Use the session number for subsequent SMC or VMC commands.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16. If the session number already exists it will be terminated and a new session initiated.

<string> Name of the calibration. Choose from:  
"VMC" or "VectorMixerCal.VMCType"  
"SMC" or "ScalarMixerCal.SMCType"

**Examples** `SENS1:CORR:COLL:SESS6:INITiate "VectorMixerCal.VMCType"`

**Query Syntax** Not Applicable

Overlapped? No

Default Not Applicable

---

**SENSe<ch>:CORRection:COLLect:SESSion<n>:SAVE?**

(Read only) Finish the SMC or VMC calibration, compute error terms, populate and save the CalSet, and return the GUID of the CalSet.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

**Examples** SENS1:CORR:COLL:SESS6:SAVE?

**Return Type** String specifying the GUID of the CalSet produced by this session.

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:CORRection:COLLect:SESSion<n>:STEPs?**

(Read-only) Returns the number of steps required by the Calibration.

To ensure this query always completes successfully, first send the write command: SENS:CORR:COLL:SESS:STEP, then send the query.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

**Examples** SENS1:CORR:COLL:SESS6:STEPs?

**Return Type** Numeric


**Overlapped?** No

**Default** Not Applicable

## Sense:Correction:Collect:Session:SMC Commands

---

Performs scalar (SMC) calibration on a frequency converting device.

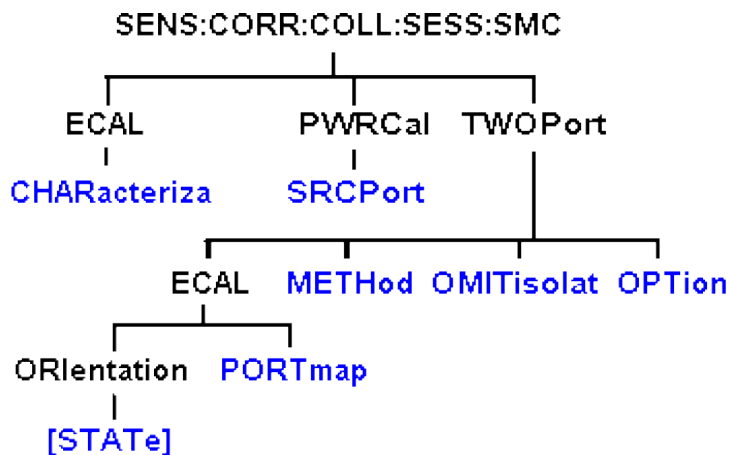

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about FCA Calibrations](#)

---

**NOTE:** To configure a power meter and sensor see [SOURCE:POWER:](#) commands.

---

### SENSe<ch>:CORRection:COLLEct:SESSion<n >:SMC:ECAL:CHARacteriza <mod> ,<char>

(Read-Write) Specifies the ECal module and characterization to be used for the SMC calibration.

#### Parameters

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

<mod> 1 - Electronic Calibration Module

<char> Specifies which characterization within the ECal module from which to read the confidence data.

0 Factory characterization (data that was stored in the ECal module by Agilent). Default if not specified.

1 User characterization #1

2 User characterization #2

3 User characterization #3

4 User characterization #4

5 User characterization #5

#### Examples

```
SENS:CORR:COLL:SESS:SMC:ECAL:CHAR 1,2
```

---

**Query Syntax** SENS:CORR:COLL:SESS:SMC:ECAL:CHAR?

**Return Type** Numeric

**Overlapped?** No

**Default** 1,0

---

## **SENSe<ch>:CORRection:COLLect:SESSion<n>:SMC:PWRCal:SRCPort <string>**

(Read-Write) Specifies which port to calibrate.

### **Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

<char> '1' Source port 1 (SMC forward direction)

'2' Source port 2 (SMC reverse direction)

'BOTH' (both forward and reverse directions)

### **Examples**

```
SENS:CORR:COLL:SESS:SMC:PWRC:SRCP 'both'
SENSe2:CORRection:COLLect:SESSion6:SMC:PWRCal:SRCPort '2'
```

**Query Syntax** SENS:CORR:COLL:SESS:SMC:PWRC:SRCP?

**Return Type** String

**Overlapped?** No

**Default** 1

---

## **SENSe<ch>:CORRection:COLLect:SESSion<n>:SMC:TWOPort:ECAL:ORlentation[:STATe] <bool>**

(Read-Write) Sets ECAL Auto-Orientation ON or OFF. If setting auto-orientation OFF, you must manually specify the orientation of the ECAL module with SENS:CORR:COLL:SESS:SMC:TWOP:ECAL:PORTmap.

#### Parameters

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16.
- <bool> **0** = Orientation OFF  
**1** = Orientation ON

#### Examples

```
SENS:CORR:COLL:SESS:SMC:TWOP:ECAL:ORI 1
```

**Query Syntax** SENS:CORR:COLL:SESS:SMC:TWOP:ECAL:ORI?

**Return Type** Boolean

**Overlapped?** No

**Default** 1

---

**SENSe<ch>:CORRection:COLLect:SESSion<n>:SMC:TWOPort:ECAL:PORTmap <mod>, <string>**

(Read-Write) Specifies the manual orientation (which ports of the module are connected to which ports of the PNA) when auto-orientation is OFF.

#### Parameters

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16.
- <mod> **1** - Electronic Calibration Module

<string> Format in the following manner:

Aw,Bx,Cy,Dz

where

- A, B, C, and D are literal ports on the ECAL module
- w,x,y, and z are substituted for PNA port numbers to which the ECAL module port is connected.

Ports of the module which are not used are omitted from the string.

**For example**, on a 4-port ECal module with

- port A connected to PNA port 2
- port B connected to PNA port 3
- port C not connected
- port D connected to PNA port 1

the string would be: A2,B3,D1

If either the receive port or source port (or load port for 2-port cal) of the CALC:PAR:SElected measurement is not in this string and orientation is OFF, an attempt to perform an ECal calibration will fail.

**Examples** `SENS:CORR:COLL:SESS:SMC:TWOP:ECAL:PORTmap 1, 'A1,B2'`

**Query Syntax** `SENS:CORR:COLL:SESS:SMC:TWOP:ECAL:PORTmap?`

**Return Type** String

**Overlapped?** No

**Default** "A1,B2"

---

**SENSe<ch>:CORRection:COLLEct:SESSion<n >:SMC:TWOPort:METHod <string>**



(Read-Write) Specifies the guided ECal method for performing the thru portion of the calibration.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

<string> ECAL Method: Choose from:

**'DEFAULT'** - Default

**'ADAP'** - Adapter removal

**'FLUSH'** - Flush Through

**'UNKN'** - Unknown Thru

**Examples**

```
SENS:CORR:COLL:SESS:SMC:TWOPort:METH 'default'
```

**Query Syntax** SENS:CORR:COLL:SESS:SMC:TWOPort:METH?

**Return Type** String

**Overlapped?** No

**Default** DEFAULT

---

**SENSe<ch>:CORRection:COLLect:SESSion<n >:SMC:TWOPort:OMITisolat <bool>**

(Read-Write) Select to omit or perform the isolation portion of the ECAL.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

<bool> **1** - Omit isolation

**0** - Perform isolation

**Examples**

```
SENS:CORR:COLL:SESS:SMC:TWOPort:OMIT 1
```

**Query Syntax** SENS:CORR:COLL:SMC:TWOPort:OMIT?

**Return Type** Boolean

**Overlapped?** No

**Default** 1

---

**SENSe<ch>:CORRection:COLLect:SESSion<n >:SMC:TWOPort:OPTion <string>**

(Read-Write) Sets the SMC calibration to ECAL or MECHANICAL

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16.

<char> Choose from:

**'ECAL'** Electronic Calibration Module

**'MECH'** Mechanical Calibration Kit

**Examples**

```
SENS:CORR:COLL:SESS:SMC:TWOPort:OPTion 'ECAL'
```

**Query Syntax**

SENS:CORR:COLL:SESS:SMC:TWOPort:OPTion?

**Return Type**

String

**Overlapped?**

No


**Default**

ECAL

## Sense:Correction:Collect:Session:VMC Commands

---

Performs a vector (VMC) calibration on a frequency converting device.

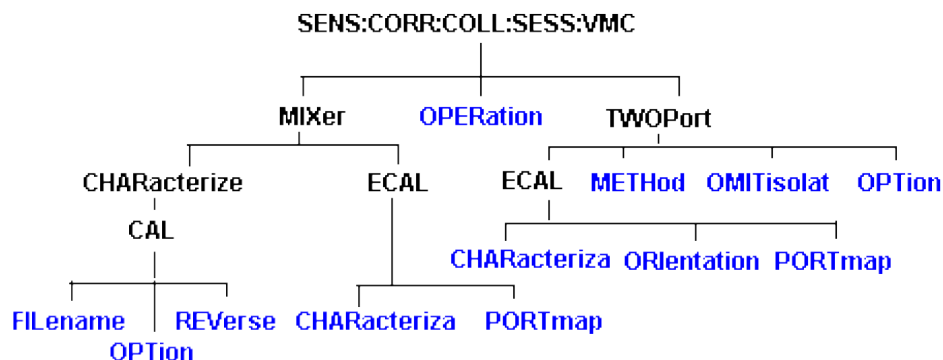

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about VMC Calibration](#)
- 


### SENS<ch>:CORREction:COLlect:SESSion<n> :VMC:CHARacterize:CAL:FILEname <string>

(Read-Write) Specifies the .S2P filename used for mixer characterization. Use the [VMC:MIXer:CHARacterize:CAL: OPTion](#) command to recall the file for mixer characterization. Once recalled, use this command to query the current filename or set a new filename.

#### Parameters

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16

 <string> Filename of the S2P used for mixer characterization. Use the full path name, file name, and .S2P suffix

#### Examples

```
SENS2:CORR:COLL:SESS4:VMC:CHAR:CAL:FILE "C:\Program
Files\Agilent\Network Analyzer\Documents\MyMixer.S2P"
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:CHAR:CAL:FIL?

**Return Type** String

**Overlapped?** No

**Default** C:\Program Files\Agilent\Network Analyzer\Documents\default.s2p

---

### SENS<ch>:CORREction:COLlect:SESSion<n> :VMC:MIXer:CHARacterize:CAL: OPTion <char>

(Read-Write) Sets the mixer characterization method to ECal, Mechanical, or read from a file.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16

<char> **ECAL** - Electronic Calibration Module

**MECH** - Mechanical Calibration Kit

**FILE, <filename>** - Retrieve a mixer characterization file. Also specify the filename of the S2P used for mixer characterization. Use the full path name, file name, and .S2P suffix. Use the VMC:CHARacterize:CAL:FILEname command to query the filename..

**Examples**

```
SENS:CORR:COLL:SESS:VMC:MIX:CHAR:CAL:OPT ECAL
SENS2:CORR:COLL:SESS6:VMC:MIXer:CHAR:CAL:OPTion FILE,
MyMixerFile.mxr
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:MIX:CHAR:CAL:OPT?

**Return Type** String

**Overlapped?** No

**Default** MECH

**SENS<ch>:CORRection:COLLect:SESSion<n> :VMC:MIXer:CHARacterize:CAL: REVerse <bool>**

(Read-Write) Specifies the direction in which to characterize the calibration mixer. [Learn more about the calibration mixer.](#)

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16

<bool> **False (0)** - Characterize the calibration mixer in the SAME direction as that specified in the mixer setup.

**True (1)** - Characterize the calibration mixer in the REVERSE direction as that specified in the mixer setup.

**Examples**

```
SENS:CORR:COLL:SESS:VMC:MIX:CHAR:CAL:REV 1
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:MIX:CHAR:CAL:REV?

**Return Type** Boolean

**Overlapped?** No

**Default** False

---

**SENS<ch>:CORREction:COLLect:SESSion<n > :VMC:MIXer:ECAL:CHARacteriza <mod>  
,<char>**

(Read-Write) Specifies the ECal module and characterization to be used for the mixer characterization portion of the calibration.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16
- <mod> 1 - Electronic Calibration Module
- <char> Characterization number in the specified ECAL module. Choose from:
  - 0 Factory characterization (data that was stored in the ECal module by Agilent). Default if not specified.
  - 1 User characterization #1
  - 2 User characterization #2
  - 3 User characterization #3
  - 4 User characterization #4
  - 5 User characterization #5

**Examples** SENS:CORR:COLL:SESS:VMC:MIX:ECAL:CHAR 1,0

**Query Syntax** SENS:CORR:COLL:SESS:VMC:MIX:ECAL:CHAR?

**Return Type** Numeric

**Overlapped?** No

**Default** 1,0

---

**SENS<ch>:CORREction:COLLect:SESSion<n> :VMC:MIXer:ECAL:PORTmap <mod>,  
<string>**

(Read-Write) Sets the port mapping for the mixer characterization with ECal. This command is required if SENS:CORR:COLL:SESS:VMC:MIX:CHAR:CAL:OPT **ECAL** is specified.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16
- <mod> **1** - Electronic Calibration Module
- <string> Choose from:
  - "A1" - ECal module port A is connected to PNA port 1
  - "B1" - ECal module port B is connected to PNA port 1

**Examples**

```
SENS:CORR:COLL:SESS:VMC:MIX:ECAL:PORT?
SENS2:CORR:COLL:SESS:VMC:MIXer:ECAL:PORTmap 1,"A1"
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:MIX:ECAL:PORTmap?

**Return Type** String

**Overlapped?** No

**Default** "A1"

---

**SENSe<ch>:CORRection:COLLect:SESSion<n>:VMC:OPERation <string>**

(Read-Write) Perform either full VMC calibration or mixer characterization only.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16
- <char> '**CAL**' - full calibration and mixer characterization  
'**CHAR**' - mixer characterization only (no reference mixer required) - Saves an .S2P file with the filename specified in SENS<ch>:CORR:COLL:SESSion<n>:VMC:CHARacterize:CAL:FILEname <filename> . If none is specified, a filename is automatically generated and can be queried using the filename command.

**Examples**

```
SENS:CORR:COLL:SESS:VMC:OPER 'CAL'
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:OPER?

**Return Type** String

**Overlapped?** No

**Default** CAL

---

**SENS<ch>:CORREction:COLLect:SESSion<n> :VMC:TWOPort:ECAL:CHARacteriza <mod>  
,<char>**

(Read-Write) Specifies the ECal module and characterization to be used for the VMC calibration.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16
- <mod> 1 - Electronic Calibration Module
- <char> Characterization number in the specified ECAL module. Choose from:
  - 0 Factory characterization (data that was stored in the ECal module by Agilent). Default if not specified.
  - 1 User characterization #1
  - 2 User characterization #2
  - 3 User characterization #3
  - 4 User characterization #4
  - 5 User characterization #5

**Examples** SENS:CORR:COLL:SESS:VMC:TWOP:ECAL:CHAR 1,1

**Query Syntax** SENS:CORR:COLL:SESS:VMC:TWOP:ECAL:CHAR?

**Return Type** Integer

**Overlapped?** No

**Default** 1,0

---

**SENS<ch>:CORREction:COLLect:SESSion<n> :VMC:TWOPort:ECAL:ORlentation[:STATe]  
<bool>**

(Read-Write) Sets ECAL orientation for the VMC ECal.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16
- <bool> **1** = ON  
**0** = OFF

**Examples**

```
SENS:CORR:COLL:SESSion:VMC:TWOPort:ECAL:ORI 1
```

**Query Syntax** SENS:CORR:COLL:SESSion:VMC:TWOPort:ECAL:ORlentation[:STATe]?

**Return Type** Integer

**Overlapped?** No

**Default** ON

**SENS<ch>:CORRection:COLLect:SESSion<n> :VMC:TWOPort:ECAL:PORTmap <mod>, <string>**

(Read-Write) Specifies the manual orientation (which ports of the module are connected to which ports of the PNA) when orientation is turned off.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <n> Session number. Choose from 1 to 16
- <mod> **1** - Electronic Calibration Module



<string> Port Map, formatted in the following manner:

**Aw,Bx,Cy,Dz**

where:

- A, B, C, and D are literal ports on the ECAL module.
- w,x,y, z are substituted for PNA port numbers to which the ECAL module port is connected.
- Ports of the module which are not used are omitted from the string.

For example, on a 4-port ECAL module with:

- port A connected to PNA port 2
- port B connected to PNA port 3
- port C not connected
- port D connected to PNA port 1

the string would be: A2,B3,D1

If either the receive port or source port (or load port for 2-port cal) of the measurement is not in this string and orientation is OFF, an attempt to perform an ECAL will fail.

**Examples**

```
SENS:CORR:COLL:SESS:VMC:TWOP:ECAL:PORTmap 1,"A2,B1"
```

**Query Syntax**

```
SENS:CORR:COLL:SESS:VMC:TWOP:ECAL:PORTmap?
```

**Return Type**

string

**Overlapped?**

No

**Default**

"A1,B2"

---

**SENS<ch>:CORRection:COLLect:SESSion<n> :VMC:TWOPort:METhod <string>**

(Read-Write) Specifies the guided ECal method for performing the thru portion of the calibration.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16

<char> **'DEFAULT'** - Default  
**'ADAP'** - Adapter removal  
**'FLUSH'** - Flush Through  
**'UNKN'** - Unknown Thru

**Examples**

```
SENS:CORR:COLL:SESS:VMC:TWOP:METH 'ADAP'
SENSe2:CORR:COLL:SESSion6:VMC:TWOPort:METHOD 'FLUSH'
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:TWOP:METH?

**Return Type** String

**Overlapped?** No

**Default** DEFAULT

---

**SENS<ch>:CORRection:COLLect:SESSion<n> :VMC:TWOPort:OMITisolat <bool>**

(Read-Write) Select to omit or perform the isolation portion of the ECAL.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16

<bool> 1 - omit isolation  
0 - perform isolation

**Examples**

```
SENS:CORR:COLL:SESS:VMC:TWOP:OMIT 1
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:TWOP:OMIT?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

**SENS<ch>:CORRection:COLLect:SESSion<n> :VMC:TWOPort:OPTion <string>**

(Read-Write) Sets the 2-port calibration option to ECAL or MECHANICAL

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1

<n> Session number. Choose from 1 to 16

<char> **Choose from:**

**'ECAL'** Electronic Calibration Module

**'MECH'** Mechanical Calibration Kit

**Examples**

```
SENS:CORR:COLL:SESS:VMC:TWOP:OPT 'MECH'
SENSe2:CORR:COLL:SESSion6:VMC:TWOPort:OPTion 'ECAL'
```

**Query Syntax** SENS:CORR:COLL:SESS:VMC:TWOP:OPT?

**Return Type** String

**Overlapped?** No

**Default** "MECH"

## Sense:Couple Commands

---

### SENSe:COUPle

PARAmeter

[STATe]

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
- 

### SENSe<cnum>:COUPle <ALL | NONE>

(Read-Write) Sets the sweep mode as Chopped or Alternate.

[Learn about Alternate Sweep](#)

#### Parameters

<cnum> Any existing channel number; if unspecified, value is set to 1.

<ALL | NONE> **ALL** - Sweep mode set to Chopped - reflection and transmission measured on the same sweep.  
**NONE** - Sweep mode set to Alternate - reflection and transmission measured on separate sweeps. Improves Mixer bounce and Isolation measurements. Increases sweep time

#### Examples

```
SENS:COUP ALL
sense2:couple none
```

**Query Syntax** SENSe<cnum>:COUPle?

**Return Type** Character

**Overlapped?** No

**Default** ALL

---

### SENSe<cnum>:COUPle:PARAmeter[:STATe] <bool>



(Read-Write) Turns ON and OFF Time Domain Trace Coupling. All of the measurements in the specified channel are coupled.

- To select Transform parameters to couple, use CALC:TRAN:COUP:PAR
- To select Gating parameters to couple, use CALC:FILT:COUP:PAR

Learn more about Time Domain Trace Coupling.

#### Parameters

<cnum> Any existing channel number; if unspecified, value is set to 1.

<bool> **ON (or 1)** - Turns ON Time Domain Trace Coupling.

**OFF (or 0)** - Turns OFF Time Domain Trace Coupling.

#### Examples

```
SENS:COUP:PAR 0
sense2:couple:parameter:state on
```

**Query Syntax** SENSE<cnum>:COUPle:PARAmeter[:STATe]?

**Return Type** Boolean

**Overlapped?** No

**Default** ON (or 1)

## Sense:Frequency Commands

---

Sets the frequency sweep functions of the analyzer.



- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - See an [example](#) using some of these commands.
  - [Learn about Frequency Sweep](#)
- 

### SENSe<num>:FREQuency:CENTer <num>

(Read-Write) Sets the center frequency of the analyzer.

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<num> Center frequency. Choose any number between the **minimum** and **maximum** frequency limits of the analyzer. Units are Hz

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

#### Examples

```
SENSe:FREQ:CENTer 1000000
sense2:frequency:center 1mhz
```

**Query Syntax** SENSe<num>:FREQuency:CENTer?



**Return Type** Numeric

**Overlapped?** No

**Default** Center of the analyzer's frequency span

---

### SENSe<num>:FREQuency[:CW |:FIXed] <num>

(Read-Write) Sets the Continuous Wave (or Fixed) frequency. Must also send SENS:SWEEP:TYPE CW to put the analyzer into CW sweep mode.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<num> CW frequency. Choose any number between the **minimum** and **maximum** frequency limits of the analyzer. Units are Hz.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See SCPI Syntax for more information.

#### Examples

```
SENS:FREQ 1000000
SENS:FREQ:CW MIN
sense2:frequency:fixed 1mhz
```

**Query Syntax** SENSE<cnum>:FREQuency[:CW | :FIXed]?

**Return Type** Numeric

**Overlapped?** No

**Default** 1 GHz

---

### SENSe<cnum>:FREQuency:SPAN <num>

(Read-Write) Sets the frequency span of the analyzer.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<num> Frequency span. Choose any number between:  
**0** (minimum) and the **maximum** frequency span of the analyzer.  
Units are Hz

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See SCPI Syntax for more information.

#### Examples

```
SENS:FREQ:SPAN 1000000
sense2:frequency:span max
```

**Query Syntax** SENSe<cnum>:FREQuency:SPAN?

**Return Type** Numeric

**Overlapped?** No

**Default** Maximum frequency span of the analyzer

---

### SENSe<cnum>:FREQuency:STARt <num>

(Read-Write) Sets the start frequency of the analyzer.

#### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <num> Start frequency. Choose any number between the **MIN** and **MAX** frequency limits of the analyzer. Units are Hz
- If `FREQ:START` is set greater than `FREQ:STOP`, then `STOP` is set equal to `START`.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
SENS:FREQ:STAR 1000000
sense2:frequency:start MIN
```

**Query Syntax** `SENSe<cnum>:FREQuency:START?`  
If [Sweep type is segment](#), this query returns the start frequency of the first segment.

**Return Type** Numeric

**Overlapped?** No

**Default** Minimum frequency of the analyzer

---

## **SENSe<cnum>:FREQuency:STOP <num>**

(Read-Write) Sets the stop frequency of the analyzer.

#### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <num> Stop frequency. Choose any number between:  
the **minimum** and **maximum** frequency limits of the analyzer. Units are Hz
- If `FREQ:STOP` is set less than `FREQ:START`, then `START` will be set equal to `STOP`.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
SENS:FREQ:STOP 1000000
sense2:frequency:stop max
```

**Query Syntax** `SENSe<cnum>:FREQuency:STOP?`  
If [Sweep type is segment](#), this query returns the stop frequency of the last segment.

**Return Type** Numeric

**Overlapped?** No

**Default** Maximum frequency of the analyzer

---






## Sense:IF Commands

---

Controls the IF source and gain settings for use with the PNA H11 Option.

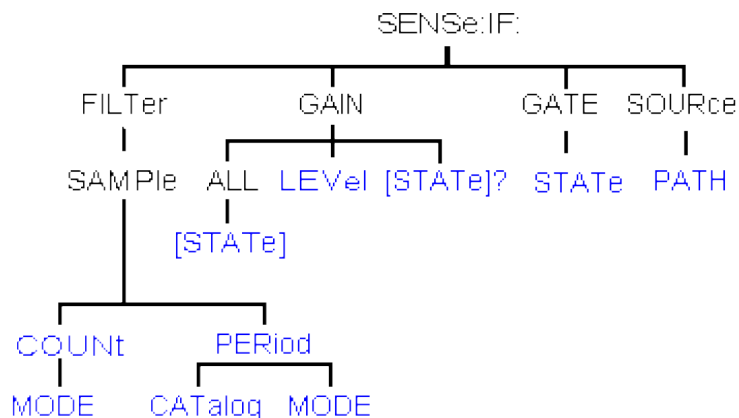

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - Learn about the [IF Access \(H11 option\)](#)
- 

### SENSe<cnUm>:IF:FILTer:SAMPle:COUNt <num>

(Read-Write) Sets and returns the number of taps in the IF filter. The IF filter sample count setting is only used when [SENSe:IF:FILTer:SAMPle:COUNt:MODE](#) is set to MANUAL. **Critical Note:**

#### Parameters

<cnUm> Existing channel number to manipulate. If unspecified, <cnUm> is set to 1.

<num> An integer value. (MIN and MAX return the minimum and maximum allowed values, respectively.)



**Examples** `SENS:IF:FILT:SAMP:COUN 40`  
`sense2:if:filter:sample:count maximum`

**Query Syntax** `SENS:IF:FILTer:SAMPle:COUNt?`

**Return Type** Numeric

**Overlapped?** No

**Default** Instrument dependent.

---

### SENSe<cnUm>:IF:FILTer:SAMPle:COUNt:MODE <char>

(Read-Write) Sets and returns the IF filter sample count mode to the specified value. When in MANUAL mode, the value specified for the IF Filter sample count is used as the number of taps in the IF filter. **Critical Note:**

**Parameters**

<cnm> Existing channel number to manipulate. If unspecified, <cnm> is set to 1.

<char> Choose either AUTO or MANUAL.

**Examples** `SENS:IF:FILT:SAMP:COUN:MODE MANUAL`  
`sense2:if:filter:sample:count:mode AUTO`

**Query Syntax** SENS:IF:FILTer:SAMPlE:COUNt:MODE?

**Return Type** Character

**Overlapped?** No

**Default** AUTO

---

**SENSe<cnm>:IF:FILTer:SAMPlE:PERiod <num>**

(Read-Write) Sets and returns the IF filter sample period. The IF filter sample period setting is only used by the instrument when the SENS:IF:FILT:SAMP:PER:MODE is set to MANUAL. **Critical Note:**

**Parameters**

<cnm> Existing channel number to manipulate. If unspecified, <cnm> is set to 1.

<num> Sample period. Choose from values returned from the SENS:IF:FILTer:SAMPlE:PERiod:CAT? command.

**Examples** `SENS:IF:FILT:SAMP:PER 6 us`  
`sense2:if:filter:sample:period maximum`

**Query Syntax** SENS:IF:FILTer:SAMPlE:PERiod?

**Return Type** Numeric

**Overlapped?** No

**Default** Instrument dependent.

---

**SENSe<cnm>:IF:FILTer:SAMPlE:PERiod:CATalog?**

(Read-Only) Returns the list of allowed IF filter sample periods for this instrument. **Critical Note:**

**Parameters**

<cnm> Existing channel number to manipulate. If unspecified, <cnm> is set to 1.

**Examples** `SENS:IF:FILT:SAMP:PER:CAT?`  
`sense2:if:filter:sample:period:catalog?`

**Query Syntax** SENS:IF:FILTer:SAMPlE:PERiod:CATalog?

**Return Type** String

**Overlapped?** No

**Default** AUTO

---

## **SENSe<cnum>:IF:FILTer:SAMPlE:PERiod:MODE <char>**

(Read-Write) Sets and returns the IF filter sample period mode to the specified value. **Critical Note:**

### **Parameters**

<cnum> Existing channel number to manipulate. If unspecified, <cnum> is set to 1.

<char> Sample period mode. Choose from **AUTO** or **MANUAL**.

### **Examples**

```
SENS:IF:FILT:SAMP:PER:MODE MANUAL
sense2:if:filter:sample:period:mode AUTO
```

**Query Syntax** SENS:IF:FILTer:SAMPlE:PERiod:MODE?

**Return Type** Character

**Overlapped?** No

**Default** AUTO

---

## **SENSe<cnum>:IF:GAIN:ALL[:STATe] <char>**

(Write only) Sets the gain state for ALL receivers to Auto or Manual.

### **Parameters**

<cnum> Existing channel number to manipulate. If unspecified, <cnum> is set to 1.

<char> Choose from **AUTO** or **MANUAL**

### **Examples**

```
SENS:IF:GAIN:ALL AUTO
sense:if:gain:all:state manual
```

**Query Syntax** Not Applicable

**Return Type** Character

**Overlapped?** No

**Default** AUTO

---

## **SENSe<cnum>:IF:GAIN:LEVEl <id>, <level>**

(Read Write) Manually sets the gain level for the specified receiver.

**Parameters**

<num> Existing channel number to manipulate. If unspecified, <num> is set to 1.

<id> Choose from: 'A', 'B', 'R1', 'R2'.

---

**Note:** The A and R1 receivers are always switched together. B and R2 are also always switched together. For example, if you specify 'A', R1 will also be switched.

---

<level> Gain level. Choose from:

0 - Lowest gain setting

1

2 - Highest gain setting

**Examples** `SENS:IF:GAIN:LEVEL 'A', 1`

**Query Syntax** `SENSe<num>:IF:GAIN:LEVEL? <id>`

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**SENSe<num>:IF:GAIN[:STATE]?, <id>**

(Read only) Returns the gain state for the specified receiver. Use `SENS:IF:GAIN:ALL` to set the gain state for all channels.

**Parameters**

<num> Existing channel number to manipulate. If unspecified, <num> is set to 1.

<id> Choose from: 'A', 'B', 'R1', 'R2'.

---

**Note:** The A and R1 receivers are always switched together. B and R2 are also always switched together. For example, if you specify 'A', R1 will also be switched.

---

**Examples** `SENS:IF:GAIN? 'A'`

**Return Type** Boolean

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<num>:IF:GATE:STATE <boolean>**

(Read-Write) Sets or returns the IF filter gate state.

**Parameters**

<num> Existing channel number to manipulate. If unspecified, <num> is set to 1.

<boolean> Choose from ON or OFF

**Examples** `SENS:IF:FILT:GATE:STAT ON`  
`sense2:if:filter:gate:state 0`

**Query Syntax** SENS:IF:FILT:er:SAMPle:COUNt:MODE?

**Return Type** Boolean

**Overlapped?** No

**Default** AUTO

---

**SENSe<num>:IF:SOURce:PATH <id>, <string>**

(Read Write) Sets the source path for the specified receiver. An error is returned if <id> is not valid, or if <char>'is not valid for the specified <id>.

**Parameters**

<num> Existing channel number to manipulate. If unspecified, <num> is set to 1.

<id> Choose from: 'A', 'B', 'R1', 'R2'

---

**Note:** The A and R1 receivers are always switched together. B and R2 are also always switched together. For example, if you specify "A", R1 will also be switched.

---

<string> Choose from:

- **'Normal'** - the PNA decides the appropriate IF input paths.
- **'External'** - always use the rear panel IF inputs.

**Examples** `SENS:IF:SOUR:PATH 'A', 'External'`

**Query Syntax** SENSe<num>:IF:SOURce:PATH? <id>

**Return Type** String


**Overlapped?** No

**Default** 'Normal'

## Sense:Mixer Commands

---

Performs Mixer setup and configuration.

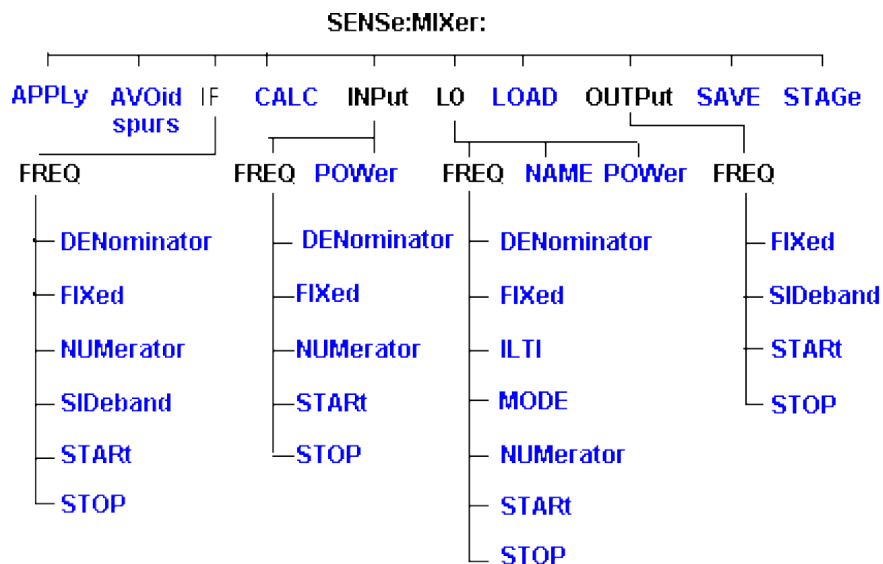

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about the Frequency Converter Application](#)

---

### SENSe<ch>:MIXer:APPLY

(Write only) Applies the mixer setup settings and turns the channel ON. (Performs the same function as the Apply button on the [mixer setup dialog box](#)).

#### Parameters



<ch> Any existing channel number. If unspecified, value is set to 1

**Examples** `SENS:MIX:APPL`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe<ch>:MIXer:AVOIdspurs <bool>

(Read Write) Sets and returns the state of the avoid spurs feature. [Learn more about avoid spurs.](#)

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <bool> Avoid spurs state. Choose from
  - 0 - Avoid spurs OFF
  - 1 - Avoid spurs ON

**Examples**

```
SENS:MIX:AVO
sense2:mixer:avoidspurs 1
```

**Query Syntax** SENSE<ch>:MIXer:AVOidspurs?

**Return Type** Boolean

**Overlapped?** No

**Default** 0 (OFF)

**SENSE<ch>:MIXer:CALCulate <char>**

(Write only) Calculates the Input, IF, or Output frequencies of the mixer setup and updates the channel settings.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1
- <char> Mixer port to be calculated. Choose from:

| <char>       | 1st or only stage requires:                                                                                                                        | In addition, 2nd stage requires:                                                                                                               |
|--------------|----------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>INPUT</b> | <ul style="list-style-type: none"><li>• Output Start and Stop frequencies</li><li>• LO frequency</li><li>• Output sideband (High or Low)</li></ul> | <ul style="list-style-type: none"><li>• IF Start and Stop frequencies</li><li>• 2nd LO frequency</li><li>• IF sideband (High or Low)</li></ul> |
| <b>Both</b>  | NA                                                                                                                                                 | <ul style="list-style-type: none"><li>• IF Start and Stop frequencies</li><li>• Both LO frequencies</li></ul>                                  |



|               |                                                                                                                                                           |                                                                                                                                                                                                                                           |
|---------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>OUTPUT</b> | <ul style="list-style-type: none"> <li>• Input Start and Stop frequencies</li> <li>• LO frequency</li> <li>• Output sideband (High or Low)</li> </ul>     | <ul style="list-style-type: none"> <li>• IF Start and Stop frequencies</li> <li>• 2nd LO frequency</li> <li>• IF sideband (High or Low)</li> </ul>                                                                                        |
| <b>LO_1</b>   | <ul style="list-style-type: none"> <li>• Input Start and Stop frequencies</li> <li>• Output frequency</li> <li>• Output sideband (High or Low)</li> </ul> | <ul style="list-style-type: none"> <li>• IF Start and Stop frequencies</li> <li>• 2nd LO frequency</li> <li>• IF sideband (High or Low)</li> </ul>                                                                                        |
| <b>LO_2</b>   | NA                                                                                                                                                        | <ul style="list-style-type: none"> <li>• Input Start and stop frequencies</li> <li>• 1st LO start and stop frequencies</li> <li>• Output frequency</li> <li>• IF sideband(High or Low)</li> <li>• Output sideband(High or Low)</li> </ul> |

**Examples** `SENS:MIX:CALC Output`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

## **SENSe<ch>:MIXer:LOAD <name>**

(Write-only) Loads a previously-configured mixer attributes file (.mxr)

### **Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<name> Path and file name (including .mxr extension) to load.

**Examples** `SENSe:MIXer:LOAD "C:\Program Files\Agilent\Network Analyzer\Documents\Mixer\MyMixer.mxr"`

**Overlapped?** No

**Default** Not Applicable

## **SENSe<ch>:MIXer:SAVE <name>**

(Write-only) Saves the settings for the mixer/converter test setup to a mixer attributes file.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<name> Path and file name (including .mxr extension) to save.

**Examples** `SENSe:MIXer:SAVE "C:\Program Files\Agilent\Network Analyzer\Documents\Mixer\MyMixer.mxr"`

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:STAGe <n>**

(Read-Write) Number of IF stages of the mixer.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<n> Number of stages. Choose either 1 or 2

**Examples** `SENSe:MIX:STAG 2`  
`SENSe:MIXer:STAGE 1`

**Query Syntax** SENSe<ch>:MIXer:STAGe?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

**SENSe<ch>:MIXer:IF:FREQuency:DENominator <num>**

(Read-Write) Sets or returns the denominator value of the IF Fractional Multiplier.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<num> Denominator value.

**Examples**

```
SENSe:MIX:IF:FREQ:DEN 5
SENSe2:MIXer:IF:FREQ:DENominator 4
```

**Query Syntax** SENSE<ch>:MIXer:IF:FREQuency:DENominator?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:IF:FREQuency:FIXed <num>**

(Read-Write) Sets or returns the fixed frequency of the IF..

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<num> Frequency.

**Examples**

```
SENSe:MIXer:IF:FREQ:FIXed 1e9
SENSe2:MIXer:IF:FREQ:FIXed 1000000000
```

**Query Syntax** SENSE<ch>:MIXer:IF:FREQuency:FIXed?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:IF:FREQuency:NUMerator <num>**

(Read-Write) Sets or returns the numerator value of the IF Fractional Multiplier.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<num> Numerator value of the IF fractional multiplier

**Examples**

```
SENSe:MIX:IF:FREQ:NUM 4
SENSe2:MIXer:IF2:FREQ:NUMerator 3
```

**Query Syntax** SENSE<ch>:MIXer:IF:FREQuency:NUMerator?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:IF:FREQuency:SIDeband <char>**

(Read-Write) Sets or returns the value of the IF sideband.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<char> Sideband value. Choose from

**LOW** - Low or Difference (-)

**HIGH** - High or Sum (+)

**Examples**

```
SENS:MIX:IF:FREQ:SIDE LOW
SENSe2:MIXer:IF:FREQ:SIDEband HIGH
```

**Query Syntax** SENSE<ch>:MIXer:IF:FREQuency:SIDeband?

**Return Type** Character

**Overlapped?** No

**Default** LOW

---

**SENSe<ch>:MIXer:IF:FREQuency:STARt <num>**

(Read-Write) Sets or returns the IF start frequency value of the mixer.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<num> IF Start Frequency value

**Examples** `SENS:MIX:IF:FREQ:STAR 1e9`  
`SENSe2:MIXer:IF:FREQ:START 1000000000`

**Query Syntax** `SENSe<ch>:MIXer:IF:FREQuency:STARt?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:IF:FREQuency:STOP <num>**

(Read-Write) Sets or returns the stop frequency value of the mixer IF frequency.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<num> IF Stop Frequency value

**Examples** `SENS:MIX:IF:FREQ:STOP 2e9`  
`SENSe2:MIXer:IF:FREQ:STOP 2000000000`

**Query Syntax** `SENSe<ch>:MIXer:IF:FREQuency:STOP?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:INPut:FREQuency:DENominator <value>**

(Read-Write) Sets or returns the denominator value of the Input Fractional Multiplier.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Input denominator value.

**Examples**

```
SENS:MIX:INP:FREQ:DEN 5
SENS2:MIXer:INPut:FREQ:DENominator 4
```

**Query Syntax** SENSE<ch>:MIXer:INPut:FREQuency:DENominator?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:INPut:FREQuency:FIXed<value>**

(Read-Write) Sets or returns the fixed frequency of the input.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Input frequency.

**Examples**

```
SENSe:MIXer:INPut:FREQ:FIXed 1e9
SENSe2:MIXer:INPut:FREQ:FIXed 1000000000
```

**Query Syntax** SENSe<ch>:MIXer:INPut:FREQuency:FIXed?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:INPut:FREQuency:NUMerator <value>**

(Read-Write) Sets or returns the numerator value of the Input Fractional Multiplier.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Input numerator value.

**Examples**

```
SENS:MIX:INP:FREQ:NUM 3
SENSe2:MIXer:INPut:FREQ:NUMerator 1
```

**Query Syntax** SENSE<ch>:MIXer:INPut:FREQ:NUMerator?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:INPut:FREQUency:STARt <value>**

(Read-Write) Sets or returns the Input start frequency value of the mixer.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Input Start frequency

**Examples**

```
SENS:MIX:INP:FREQ:STAR 1e9
SENSe2:MIXer:INPut:FREQ:STARt 1000000000
```

**Query Syntax** SENSE<ch>:MIXer:INPut:FREQUency:STARt?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:INPut:FREQUency:STOP <value>**

(Read-Write) Sets or returns the Input stop frequency value of the mixer.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Input stop frequency

**Examples**

```
SENS:MIX:INP:FREQ:STOP 2e9
SENSe2:MIXer:INPut:FREQ:STOP 2000000000
```

**Query Syntax** SENSE<ch>:MIXer:INPut:FREQuency:STOP?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:INPut:POWer <value>**

(Read-Write) Sets or returns the value of the Input Power.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Input power in dBm.

**Examples**

```
SENS:MIX:INP:POW 9
SENSe2:MIXer:INPut:POWer 5
```

**Query Syntax** SENSE<ch>:MIXer:INPut:POWer?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:LO<n>:FREQuency:DENominator <value>**



(Read-Write) Sets or returns the denominator value of the LO Fractional Multiplier.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose 1 or 2.
- <value> LO denominator.

**Examples**

```
SENS:MIX:LO:FREQ:DEN 5
SENSe2:MIXer:LO2:FREQ:DENominator 4
```

**Query Syntax** SENSE<ch>:MIXer:LO<n>:FREQuency:DENominator?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

**SENSe<ch>:MIXer:LO<n>:FREQuency:FIXed <value>**

(Read-Write) Sets or returns the fixed frequency of the specified mixer LO.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose 1 or 2
- <value> LO frequency.

**Examples**

```
SENS:MIX:LO:FREQ:FIX 1e9
SENSe2:MIXer:LO2:FREQ:FIXed 1000000000
```

**Query Syntax** SENSE<ch>:MIXer:LO<n>:FREQuency:FIXed?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:LO<n>:FREQuency:ILTI <bool>**

(Read-Write) Specifies whether to use the Input frequency that is **greater than** the LO or **less than** the LO. To learn more, see the [mixer setup](#) dialog box help.

#### Parameters

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose **1** or **2**
- <bool> **True (1)** - Use the Input that is Greater than the specified LO.  
**False (0)** - Use the Input that is Less than the specified LO.

#### Examples

```
SENS:MIX:LO1:FREQ:ILTI 1
sense2:mixer:lo2:frequency:ilti true
```

**Query Syntax** SENSE<ch>:MIXer:LO<n>:FREQUency:ILTI?

**Return Type** Boolean

**Overlapped?** No

**Default** False

---

### SENSE<ch>:MIXer:LO<n>:FREQUency:MODE <char>

(Read-Write) Sets or returns the LO sweep mode.

#### Parameters

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose **1** or **2**
- <char> LO sweep mode. Choose either **FIXED** or **SWEPT**

#### Examples

```
SENS:MIX:LO:FREQ:MODE FIXED
SENSE2:MIXer:LO2:FREQ:MODE swept
```

**Query Syntax** SENSE<ch>:MIXer:LO<n>:FREQUency:MODE?

**Return Type** Character

**Overlapped?** No

**Default** Fixed

---

### SENSE<ch>:MIXer:LO<n>:FREQUency:NUMerator <value>

(Read-Write) Sets or returns the numerator value of the LO Fractional Multiplier.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose 1 or 2
- <value> LO Numerator.

**Examples**

```
SENS:MIX:LO:FREQ:NUM 5
SENSe2:MIXer:LO2:FREQ:NUMerator 4
```

**Query Syntax** SENSE<ch>:MIXer:LO<n>:FREQuency:NUMerator?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:LO<n>:FREQuency:STARt <value>**

(Read-Write) Sets or returns the LO start frequency value. This command can only be used with SMC (not VMC) measurements.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose 1 or 2
- <value> LO Start Frequency in Hertz.

**Examples**

```
SENS:MIX:LO:FREQ:STAR 5E9
```

**Query Syntax** SENSE<ch>:MIXer:LO<n>:FREQuency:STARt?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:LO<n>:FREQuency:STOP <value>**

(Read-Write) Sets or returns the LO stop frequency value. This command can only be used with SMC (not VMC) measurements.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose **1** or **2**
- <value> LO Stop Frequency in Hertz.

**Examples** `SENS:MIX:LO:FREQ:STOP 5E9`

**Query Syntax** `SENSe<ch>:MIXer:LO<n>:FREQuency:STOP?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:LO<n>:NAME <value>**

(Read-Write) Sets or returns the name of the external LO source.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage number. Choose 1 or 2.
- <value> External LO source name

**Examples** `SENS:MIX:LO:NAME "MySource"`

**Query Syntax** `SENSe<ch>:MIXer:LO<n>:NAME?`

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:LO<n>:POWER <value>**

(Read-Write) Sets or returns the value of the LO Power.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <n> LO stage. Choose **1** or **2**
- <value> LO Power in dBm

**Examples** `SENS:MIX:LO:POW 9`

**Query Syntax** `SENSe<ch>:MIXer:LO<n>:POWer?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:OUTPut:FREQuency:FIXed <value>**

(Read-Write) Sets or returns the output fixed frequency of the mixer. This command can only be used with SMC (not VMC) measurements.

**Parameters**

- <ch> Any existing channel number. If unspecified, value is set to 1.
- <value> Output fixed frequency in Hertz.

**Examples** `SENS:MIX:OUTP:FREQ:FIX 5e9`

**Query Syntax** `SENSe<ch>:MIXer:OUTPut:FREQuency:FIXed?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:OUTPut:FREQuency:SIDeband <value>**

(Read-Write) Sets or returns the value of the output sideband.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> **Boolean** Sideband value. Choose from

**LOW** - Low or Difference (-)

**HIGH** - High or Sum (+)

**Examples**

```
SENS:MIX:OUTP:FREQ:SIDE LOW
SENSe2:MIXer:OUTPut:FREQ:SIDeband HIGH
```

**Query Syntax** SENSE<ch>:MIXer:OUTPut:FREQuency:SIDeband?

**Return Type** Character

**Overlapped?** No

**Default** LOW

---

**SENSe<ch>:MIXer:OUTPut:FREQuency:STARt <value>**

(Read-Write) Sets or returns the Output start frequency of the mixer.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Output start frequency

**Examples**

```
SENS:MIX:OUTP:FREQ:STAR 1e9
SENSe2:MIXer:OUTPut:FREQ:STARt 1000000000
```

**Query Syntax** SENSE<ch>:MIXer:OUTPut:FREQuency:STARt?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSe<ch>:MIXer:OUTPut:FREQuency:STOP <value>**

(Read-Write) Sets or returns the Output stop frequency of the mixer.

**Parameters**

<ch> Any existing channel number. If unspecified, value is set to 1.

<value> Output stop frequency

**Examples**

```
SENS:MIX:OUTP:FREQ:STOP 1e9
SENSe2:MIXer:OUTPut:FREQ:STOP 1000000000
```

**Query Syntax** SENSE<ch>:MIXer:OUTPut:FREQuency:STOP?

**Return Type** Numeric

**Overlapped?** No


**Default** Not Applicable

---

## Sense:Offset Commands

---

Sets the offset frequency functions, causing the stimulus and response frequencies to be different.



- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Frequency Offset](#)
- 

### SENSe<num>:OFFSet:CW <bool>

(Read-Write) Turns stimulus CW Override mode ON or OFF. Use this setting to establish a fixed (CW) stimulus frequency while measuring the Response over a swept frequency range. [Learn more about Frequency Offset.](#)

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<bool> ON (or 1) - turns CW override ON.  
OFF (or 0) - turns CW override OFF.

#### Examples

```
SENS:OFFS:CW ON
sense2:offset:cw off
```

**Query Syntax** SENSE<num>:OFFSet:CW?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF



---

### SENSe<num>:OFFSet:DIVisor <num>



(Read-Write) Specifies (along with the multiplier) the value to multiply by the stimulus. [Learn more about Frequency Offset.](#)

#### Parameters

<cnm> Any existing channel number. If unspecified, value is set to 1

<num> Divisor value. Range is 1 to 1000

**Examples** `SENS:OFFS:DIV 3`  
`sense2:offset:divisor 2`

**Query Syntax** SENSE<cnm>:OFFSet:DIVisor?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

#### SENSe<cnm>:OFFSet:MULTiplier <num>

(Read-Write) Specifies (along with the divisor) the value to multiply by the stimulus. [Learn more about Frequency Offset.](#)

#### Parameters

<cnm> Any existing channel number. If unspecified, value is set to 1

<num> Multiplier value. Range is +/- 1000. Negative multipliers cause the stimulus to sweep in decreasing direction. For mixer measurements, this would be for setups requiring the RF frequency to be less than LO frequency

**Examples** `SENS:OFFS:MULT 2`  
`sense2:offset:multipier 4`

**Query Syntax** SENSe<cnm>:OFFSet:MULTplier?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

#### SENSe<cnm>:OFFSet:OFFSet <num>

(Read-Write) Specifies an absolute offset frequency in Hz. For mixer measurements, this would be the LO frequency. [Learn more about Frequency Offset.](#)

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <num> Offset frequency. Range is +/- 1000 GHz. Offsets can be positive or negative

**Examples** `SENS:OFFS:OFFS 1GHz`  
`sense2:offset:offset 1e9`

**Query Syntax** SENSE<num>:OFFSet:OFFSet?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 Hz

---

**SENSe<num>:OFFSet:STARt?**

(Read-Only) Returns the response start frequency [Learn more about Frequency Offset.](#)

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1

**Examples** `SENS:OFFS:STAR?`  
`sense2:offset:start?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not applicable

---

**SENSe<num>:OFFSet:[STATe] <bool>**

(Read-Write) Enables Frequency Offset Mode on ALL measurements that are present on the active channel. This immediately causes the source and receiver to tune to separate frequencies. The receiver frequencies are specified with the other SENS:OFFSet commands. To make the stimulus settings use the [SENS:FREQ](#) commands.

Tip: To avoid unnecessary errors, first make other offset frequency settings, then set Frequency Offset ON. [Learn more about Frequency Offset.](#)

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<bool> ON (or 1) - turns Frequency Offset ON.  
OFF (or 0) - turns Frequency Offset OFF.

#### Examples

```
SENS:OFFS ON
sense2:offset:state off
```

**Query Syntax** SENSE<num>:OFFSet:[STATe]?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF (0)

---

### SENSe<num>:OFFSet:STOP?

(Read-Only) Returns the response stop frequency. [Learn more about Frequency Offset.](#)

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

#### Examples

```
SENS:OFFS:STOP
sense2:offset:stop
```

**Return Type** Numeric

**Overlapped?** No

**Default** Not applicable

## Sense:Power Command

---

[Learn about Receiver Attenuation](#)

### **SENSe<num>:POWER:ATTenuation <recvr>,<num>**

(Read-Write) Sets the attenuation level for the specified receiver.

---

**Note:** Attenuation cannot be set with Sweep Type set to Power

---

#### Parameters

- <num> Any existing channel number. If unspecified, value is set to 1
- <recvr> Receiver to get attenuation. Choose from:  
**ARECeiver** - receiver A  
**BRECeiver** - receiver B
- <num> Choose from:  
**0** to **35** dB - in 5 dB steps  
If a number other than these is entered, the analyzer will select the next lower valid value. For example, if 19.9 is entered for <num> the analyzer will switch in 15 dB attenuation.

#### Examples

```
SENS:POW:ATT AREC,10
sense2:power:
 attenuation breceiver,30
```

**Query Syntax** SENSe<num>:POWER:ATTenuation? <rec>

**Return Type** Numeric

**Overlapped?** No

**Default** 0



## Sense:Roscillator Command

---

[Learn about the Reference Osc.](#)

### SENSe:ROSCillator:SOURce?

(Read-only) Applying a signal to the Reference Oscillator connector automatically sets the Reference Oscillator to EXTERNAL. This command allows you to check that it worked.

**EXT** is returned when a signal is present at the **Reference Oscillator** connector.

**INT** is returned when **NO** signal is present at the **Reference Oscillator** connector.

|                 |                                                                        |
|-----------------|------------------------------------------------------------------------|
| <b>Examples</b> | <code>SENS:ROSC:SOUR?</code><br><code>sense:roscillator:source?</code> |
|-----------------|------------------------------------------------------------------------|

**Return Type** Character

**Overlapped?** No

**Default** Not applicable


---



## Sense:Segment Commands

---

Defines the segment sweep settings. Enable segment sweep with **SENS:SWE:TYPE SEGMENT**.

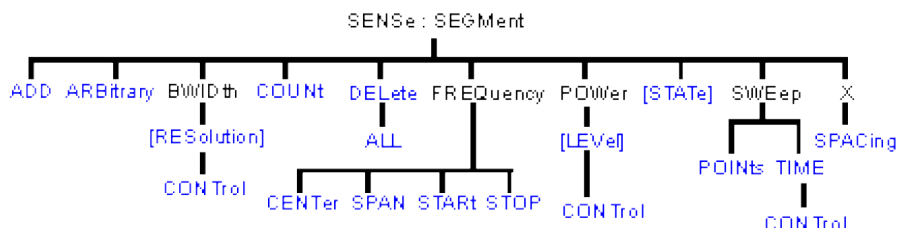

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Segment Sweep](#)
- 

### SENSe<cnUm>:SEGMENT<snUm>:ADD

(Write-only) Adds a segment.

#### Parameters

- <cnUm> Any existing channel number. If unspecified, value is set to 1
- <snUm> Segment number to add. If unspecified, value is set to 1. Segment numbers must be sequential. If a new number is added where one currently exists, the existing segment and those following are incremented by one.

#### Examples

Two Segments exist (1 and 2). The following command will add a new segment (1). The existing (1 and 2) will become (2 and 3) respectively.

```
SENSe:SEGMENT1:ADD
sense2:segment1:add
```



**Query Syntax** Not applicable. Use Sense:Segment:Count to determine the number of segments in a trace.

**Overlapped?** No

**Default** Not Applicable

---

### SENSe<cnUm>:SEGMENT:ARBITRARY <ON | OFF>

(Read-Write) Enables you to setup a segment sweep with arbitrary frequencies. The start and stop frequencies of each segment can overlap other segments. Also, each segment can have a start frequency that is greater than its stop frequency which causes a reverse sweep over that segment. Learn more about [Arbitrary Segment Sweep](#).

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1.

<ON | OFF> **ON** (or 1) - Allows the setup of arbitrary segment sweep.  
**OFF** (or 0) - Prevents the setup of arbitrary segment sweep.

#### Examples

```
SENS:SEGM:ARB ON
sense2:segment:arbitrary off
```

**Query Syntax** SENSE<cnum>:SEGMENT:ARbitrary?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

### SENSE<cnum>:SEGMENT<snum>:BWIDth[:RESolution] <num>

(Read-Write) Sets the IF Bandwidth for the specified segment. First set SENS:SEGM:BWIDth:CONTROL ON. All subsequent segments that are added assume the new IF Bandwidth value.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<snum> Segment number to modify. Choose any existing segment number.

<num> IF Bandwidth in Hz. The list of valid IF Bandwidths is different depending on the PNA model. ([Click to see the lists.](#)) If an invalid number is specified, the analyzer will round up to the closest valid number.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

#### Examples

```
SENS:SEGM:BWID 1KHZ
sense2:segment2:bwid:resolution max
```

**Query Syntax** SENSE<cnum>:SEGMENT<snum>:BWIDth[:RESolution]?

**Return Type** Numeric

**Overlapped?** No

**Default** See [Preset IFBW](#) for your PNA model.

---

### SENSE<cnum>:SEGMENT:BWIDth[:RESolution]:CONTROL <ON | OFF>

(Read-Write) Specifies whether the IF Bandwidth resolution can be set independently for each segment.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns Bandwidth control ON. Bandwidth can be set for each segment  
**OFF** (or 0) - turns Bandwidth control OFF. Use channel bandwidth setting

**Examples**

```
SENS:SEGM:BWID:CONT ON
sense2:segment:bandwidth:control off
```

**Query Syntax** SENSE<cnum>:SEGMENT:BWIDth[:RESolution]:CONTROL?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**SENSe<cnum>:SEGMENT:COUNT?**

(Read-only) Queries the number of segments that exist in the specified channel.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

**Examples**

```
SENS:SEGM:COUNT?
sense2:segment:count?
```

**Return Type** Numeric

**Overlapped?** No

**Default** 1 segment

---

**SENSe<cnum>:SEGMENT<snum>:DELETE**



(Write-only) Deletes the specified sweep segment.

<cnum> Any existing channel number. If unspecified, value is set to 1

<snum> Number of the segment to delete. If unspecified, value is set to 1

**Examples** `SENS:SEGM:DEL`  
`sense2:segment2:delete`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe<cnum>:SEGMENT:DELeTE:ALL

(Write-only) Deletes all sweep segments.

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

**Examples** `SENS:SEGM:DEL:ALL`  
`sense2:segment:delete:all`

**Query Syntax** Not applicable

**Overlapped?** No

**Default** Not Applicable

---

### SENSe<cnum>:SEGMENT<snum>:FREQUency:CENTer <num>

(Read-Write) Sets the Center Frequency for the specified segment. The Frequency Span of the segment remains the same. The Start and Stop Frequencies change accordingly.

**Note:** All previous segment's Start and Stop Frequencies that are larger than the new Start Frequency are changed to the new Start Frequency. All following segment's start and stop frequencies that are smaller than the new Stop Frequency are changed to the new Stop Frequency.

---

#### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<snum> Segment number to modify. Choose any existing segment number.

<num> Center Frequency in Hz. Choose any number between the **minimum** and **maximum** frequency of the analyzer.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
SENS:SEGM:FREQ:CENT 1MHZ
sense2:segment2:frequency:center 1e9
```

**Query Syntax** SENSE<cnum>:SEGMENT<snum>:FREQUENCY:CENTER?

**Return Type** Numeric

**Overlapped?** No

**Default** Stop Frequency of the previous segment. If first segment, start frequency of the analyzer.

---

## SENSE<cnum>:SEGMENT<snum>:FREQUENCY:SPAN <num>

(Read-Write) Sets the Frequency Span for the specified segment. The center frequency of the segment remains the same. The start and stop frequencies change accordingly.

**Note:** All previous segment's Start and Stop Frequencies that are larger than the new Start Frequency are changed to the new Start Frequency. All following segment's start and stop frequencies that are smaller than the new Stop Frequency are changed to the new Stop Frequency.

---

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<snum> Segment number to modify. Choose any existing segment number.

<num> Frequency Span in Hz. Choose any number between the **minimum** and **maximum** frequency of the analyzer.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
SENS:SEGM:FREQ:SPAN 1MHZ
sense2:segment2:frequency:span max
```

**Query Syntax** SENSE<cnum>:SEGMENT<snum>:FREQUENCY:SPAN?

**Return Type** Numeric

**Overlapped?** No

**Default** If first segment, frequency span of the analyzer. Otherwise 0.

---

## SENSE<cnum>:SEGMENT<snum>:FREQUENCY:START <num>

(Read-Write) Sets the Start Frequency for the specified sweep segment.

### Notes

All other segment Start and Stop Frequency values that are larger than this frequency are changed to this frequency.

To return the start and stop frequency of the entire sweep (all segments), Use [SENS:FREQ:START?](#) and [SENS:FREQ:STOP?](#)

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <snum> Segment number to modify. Choose any existing segment number.
- <num> Start Frequency in Hz. Choose any number between the **minimum** and **maximum** frequency of the analyzer.

---

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

### Examples

```
SENS:SEGM:FREQ:STAR 1MHZ
sense2:segment2:frequency:start minimum
```

**Query Syntax** SENSE<cnum>:SEGMENT<snum>:FREQUENCY:STAR?

**Return Type** Numeric

**Overlapped?** No

**Default** Stop Frequency of the previous segment. If first segment, start frequency of the analyzer.

---

## SENSe<cnum>:SEGMENT<snum>:FREQUENCY:STOP <num>

(Read-Write) Sets the Stop Frequency for the specified sweep segment.

### Notes

All other segment Start and Stop Frequency values that are larger than this frequency are changed to this frequency.

To return the start and stop frequency of the entire sweep (all segments), Use [SENS:FREQ:START?](#) and [SENS:FREQ:STOP?](#)

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <snum> Segment number to modify. Choose any existing segment number.
- <num> Stop Frequency in Hz. Choose any number between the **minimum** and **maximum** frequency of the analyzer.

---

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
SENS:SEGM:FREQ:STOP 1MHZ
sense2:segment2:frequency:stop maximum
```

**Query Syntax** SENSE<cnum>:SEGMENT<snum>:FREQUENCY:STOP?

**Return Type** Numeric

**Overlapped?** No

**Default** If first segment, stop frequency of the analyzer. Otherwise, start frequency of the segment.

## SENSE<cnum>:SEGMENT<snum>:POWER[<port>][:LEVEL] <num>

(Read-Write) Sets the Port Power level for the specified sweep segment. First set SENS:SEGM:POW:CONTROL ON.

All subsequent segments that are added assume the new Power Level value.

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <snum> Segment number to modify. Choose any existing segment number.
- <port> Port number of the source. Choose from 1 or 2. If unspecified, value is set to 1.
- <num> Power level.

**Note:** The range of settable power values depends on the PNA model and if source attenuators are installed. To determine the range of values, send SOUR:POW? MAX and SOUR:POW? MIN. (SOUR:POW:ATT:AUTO must be set to ON).

Actual achievable leveled power depends on frequency.

**Examples**

```
SENS:SEGM:POW 0
sense2:segment2:power1:level -10
```

**Query Syntax** SENSE<cnum>:SEGMENT<snum>:POWER[<port>][:LEVEL]?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

## SENSE<cnum>:SEGMENT:POWER[:LEVEL]:CONTROL <ON | OFF>

(Read-Write) Specifies whether Power Level can be set independently for each segment.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns Power Level control ON. Power level can be set for each segment.  
**OFF** (or 0) - turns Power Level control OFF. Use the channel power level setting.

**Examples**

```
SENS:SEGM:POW:CONT ON
sense2:segment:power:level:control off
```

**Query Syntax** SENSE<cnum>:SEGMENT:POWER[:LEVEL]:CONTROL?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**SENSE<cnum>:SEGMENT<snum>[:STATE] <ON | OFF>**

(Read-Write) Turns the specified sweep segment ON or OFF.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<snum> Segment number to be turned ON or OFF

<ON | OFF> **ON** (or 1) - turns segment ON.  
**OFF** (or 0) - turns segment OFF.

**Examples**

```
SENS:SEGM ON
sense2:segment2:state off
```

**Query Syntax** SENSE<cnum>:SEGMENT[:STATE]? <snum>

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**SENSE<cnum>:SEGMENT<snum>:SWEep:POINTs <num>**

(Read-Write) Sets the number of data points for the specified sweep segment.

**Parameters**

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <snum> Any existing segment number. If unspecified, value is set to 1
- <num> Number of points in the segment. The total number of points in all segments cannot exceed **16001**. A segment can have as few as 1 point.

---

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
SENS:SEGM:SWE:POIN 51
sense2:segment2:sweep:points maximum
```

**Query Syntax** SENSE<cnm>:SEGMent<snum>:SWEep:POINTs?

**Return Type** Numeric

**Overlapped?** No

**Default** 201

---

**SENSE<cnm>:SEGMent<snum>:SWEep:TIME <num>**

(Read-Write) Sets the time the analyzer takes to sweep the specified sweep segment.

**Parameters**

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <snum> Any existing segment number.
- <num> Sweep time in seconds. Choose a number between **0** and **100**

---

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

**Examples**

```
SENS:SEGM:SWE:TIME 1ms
sense2:segment2:sweep:time .001
```

**Query Syntax** SENSE<cnm>:SEGMent<snum>:SWEep:TIME?

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

**SENSE<cnm>:SEGMent:SWEep:TIME:CONTrol <ON | OFF>**

(Read-Write) Specifies whether Sweep Time can be set independently for each sweep segment.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns Sweep Time control ON. Sweep Time can be set for each segment.  
**OFF** (or 0) - turns Sweep Time control OFF. Uses the channel Sweep Time setting.

**Examples**

```
SENS:SEGM:SWE:TIM:CONT ON
sense2:segment:sweep:time:control off
```

**Query Syntax** SENSE<cnum>:SEGMENT:SWEep:TIME:CONTROL?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**SENSe<cnum>:SEGMENT<snum>:X:SPACing <char>**

(Read-Write) Sets X-axis spacing ON or OFF

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<snum> Any existing segment number. (This parameter is ignored)

<char> **LINear** - turns X-axis point spacing OFF  
**OBASe** - turns X-axis point spacing ON

**Examples**

```
SENS:SEGM:X:SPACing LIN
sense2:segment1:spacing obase
```

**Query Syntax** SENSe<cnum>:SEGMENT<snum>:X:SPACing?

**Return Type** Character

**Overlapped?** No


**Default** LINear

---

## Sense:Sweep Commands

---

Specifies the sweep functions of the analyzer.

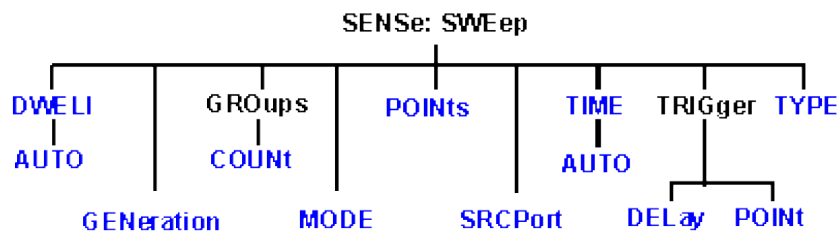

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Sweeping](#)
- 

### SENSe<cnun>:SWEEp:DWELI <num>

(Read-Write) Sets the dwell time between each sweep point.

- Dwell time is **ONLY** available with SENSE:SWEEP:GENERATION set to **STEPped**; It is **Not** available in **ANALOG**.
- Sending dwell = 0 is the same as setting SENSE:SWEEP:DWELI:AUTO **ON**. Sending a dwell time > 0 sets SENSE:SWEEP:DWELI:AUTO **OFF**.

#### Parameters

<cnun> Any existing channel number. If unspecified, value is set to 1

<num> Dwell time in seconds.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.



#### Examples

```
SENSe:SWEEP:DWELI .1
sense2:sweep:dwell min
```

**Query Syntax** SENSE<cnun>:SWEEP:DWELI?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 - (**Note:** dwell time set to 0 is the same as dwell:auto ON)

---

### SENSe<cnun>:SWEEP:DWELI:AUTO <ON | OFF>



(Read-Write) Specifies whether or not to automatically calculate and set the minimum possible dwell time. Setting Auto **ON** has the same effect as setting dwell time to **0**.

**Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns dwell ON.  
**OFF** (or 0) - turns dwell OFF.

**Examples** `SENS:SWE:DWEL:AUTO ON`  
`sense2:sweep:dwell:auto off`

**Query Syntax** SENSE<num>:SWEep:DWELI:AUTO?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

**SENSe<num>:SWEep:GENeration <char>**

(Read-Write) Sets sweep as Stepped or Analog.

**Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<char> Choose from:

**STEPped** - source frequency is CONSTANT during measurement of each displayed point. More accurate than ANALog. Dwell time can be set in this mode.

**ANALog** - source frequency is continuously RAMPING during measurement of each displayed point. Faster than STEPped. Sweep time (not dwell time) can be set in this mode.

**Examples** `SENS:SWE:GEN STEP`  
`sense2:sweep:generation analog`

**Query Syntax** SENSE<num>:SWEep:GENeration?

**Return Type** Character

**Overlapped?** No

**Default** Analog

---

**SENSe<num>:SWEep:GROups:COUNT <num>**

(Read-Write) Sets the trigger count (groups) for the specified channel. Set trigger mode to group after setting this count.

**Parameters**

- <cnnum> Any existing channel number. If unspecified, value is set to 1
- <num> Count (groups) number. Choose any number between: **1** and **2e6** (1 is the same as single trigger)

**Examples**

```
SENS:SWE:GRO:COUN 10
sense2:sweep:groups:count 50
```

**Query Syntax** SENSE<cnnum>:SWEep:GROups:COUNT?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

**SENSe<cnnum>:SWEep:MODE <char>**

(Read-Write) Sets the trigger mode for the specified channel.

**Parameters**

- <cnnum> Any existing channel number. If unspecified, value is set to 1
- <char> Trigger mode. Choose from:
  - HOLD** - channel will not trigger
  - CONTInuous** - channel triggers indefinitely
  - GROups** - channel accepts the number of triggers specified with the last SENS:SWE:GRO:COUN <num>

**Examples**

```
SENS:SWE:MODE CONT
sense2:sweep:mode hold
```

**Query Syntax** SENSE<cnnum>:SWEep:MODE?

**Return Type** Character

**Overlapped?** **YES** - SENS:SWE:MODE GROUPS (when INIT:CONT is ON)  
**NO** - HOLD and CONTInuous

**Default** CONTInuous

---

**SENSe<cnnum>:SWEep:POINTs <num>**

(Read-Write) Sets the number of data points for the measurement.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<num> Choose any number between 1 and 16001

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

**Examples**

```
SENS:SWE:POIN 51
sense2:sweep:points max
```

**Query Syntax** SENSE<cnum>:SWEep:POINTs?

**Return Type** Numeric

**Overlapped?** No

**Default** 201

---

**SENSe<cnum>:SWEep:SRCPort <1 | 2>**

(Read-Write) Sets the source port when making non S-parameter measurements. Has no effect on S-parameter measurements.

**Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<1 | 2> 1 - Source power comes out Port 1  
2 - Source power comes out Port 2

**Examples**

```
SENS:SWE:SRCP 1
sense2:sweep:srcport 2
```

**Query Syntax** SENSe<cnum>:SWEep:SRCPort?

**Return Type** Character

**Overlapped?** No

**Default** 1

---

**SENSe<cnum>:SWEep:TIME <num>**

(Read-Write) Sets the time the analyzer takes to complete one sweep. If sweep time accuracy is critical, use ONLY the values that are attained using the up and down arrows next to the sweep time entry box. [See Sweep Time.](#)

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<num> Sweep time in seconds. Choose a number between **0** and **86,400** (24hrs),  
To select the fastest sweep speed, either send MIN as an argument to this command, or send SENS:SWE:TIME:AUTO 1

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

#### Examples

```
SENS:SWE:TIME 1ms
sense2:sweep:time .001
```

**Query Syntax** SENSE<num>:SWEep:TIME?

**Return Type** Numeric

**Overlapped?** No

**Default** NA

---

### SENSe<num>:SWEep:TIME:AUTO <ON | OFF>

(Read-Write) Turns the automatic sweep time function ON or OFF.

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns the automatic sweep time ON.  
**OFF** (or 0) - turns the automatic sweep time OFF.

#### Examples

```
SENS:SWE:TIME:AUTO
sense2:sweep:time:auto off
```

**Query Syntax** SENSE<num>:SWEep:TIME:AUTO?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

### SENSe<num>:SWEep:TRIGger:DElay <num>

(Read-Write) Sets and reads the trigger delay for all measurements in the specified CHANNEL. This delay is only applied while TRIG:SOURce EXTERNAL and TRIG:SCOPE CURRENT. After an external trigger is applied, the start of the sweep is delayed for the specified delay value plus any inherent latency.

To apply a trigger delay for all channels (Global), use TRIG:DEL

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <num> Trigger delay value in seconds. Range is from 0 to 107 seconds

**Examples** `SENS:SWE:TRIG:DELAY .003`  
`sense2:sweep:trigger:delay 1`

**Query Syntax** `SENSe<num>:SWEep:TRIGger:DELay?`

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**SENSe<num>:SWEep:TRIGger:POINT <ON | OFF>**

(Read-Write) Specifies whether the specified channel will measure one point for each trigger or all of the measurements in the channel. Setting any channel to POINT mode will automatically set the TRIGger:SCOPE = CURRENT.

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <ON | OFF> **ON** (or 1) - Channel measures one data point per trigger.  
**OFF** (or 0) - All measurements in the channel made per trigger.

**Examples** `SENS:SWE:TRIG:POINT ON`  
`sense2:sweep:trigger:point off`

**Query Syntax** `SENSe<num>:SWEep:TRIGger:POINT?`

**Return Type** Boolean (1 = Point, 0 = Measurement)

**Overlapped?** No

**Default** 0 - Measurement

---

**SENSe<num>:SWEep:TYPE <char>**

(Read-Write) Sets the type of analyzer sweep mode.

**Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<char> Choose from:

**LINear | LOGarithmic | POWer | CW | SEGMENT**

---

**Note:** SWEep TYPE cannot be set to SEGMENT if there are no segments turned ON. A segment is automatically turned ON when the analyzer is started.

---

**Examples**

```
SENS:SWE:TYPE LIN
sense2:sweep:type segment
```

**Query Syntax** SENSE<num>:SWEep:TYPE?

**Return Type** Character

**Overlapped?** No

**Default** LINear

## X Values Command

---

### SENSe<num>:X[:VALues]?

(Read-only) Returns the stimulus values for the specified channel. If the channel is sweeping the source backwards, the values will be in descending order.

#### Parameters

<num> Any existing channel number; if unspecified, value is set to 1.

#### Examples

```
SENS:X?
sense2:x:values?
```

**Return Type** Depends on FORM:DATA command


**Overlapped?** No

**Default** Not applicable

## Source Commands

---

Controls the power delivered to the DUT.

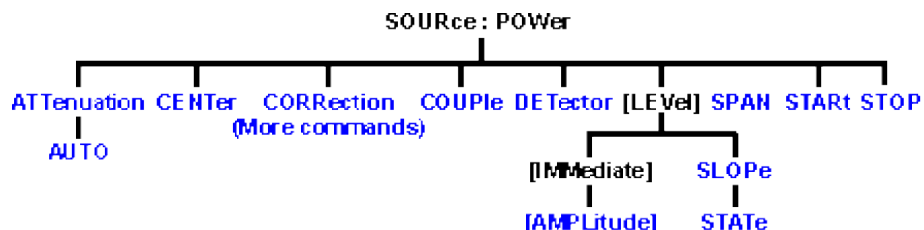

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Power Settings](#)
- 

### SOURce<cnum>:POWER<port>:ATTenuation <num>

(Read-Write) Sets the attenuation level for the selected channel. Sending this command turns automatic attenuation control (SOUR:POW:ATT:AUTO) to OFF. If the ports are coupled, changing the attenuation on one port will also change the attenuation on the other port. To turn port coupling OFF use SOURce:POWER:COUPlE OFF.

**Note:** Attenuation cannot be set with **Sweep Type** set to **Power**

---

#### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <port> Port number of the attenuator being set. Choose 1 or 2; If unspecified, value is set to 1.
- <num> Attenuation value. The range of settable values depends on the PNA model. To determine the range of values, perform a query using MAX, then MIN, as an argument. Example: SOURce:POWER:ATT? Max

Enter a value between MAX and MIN in 10 dB steps.

If a number other than these is entered, the analyzer will select the next lower valid value. For example, if 19.9 is entered for <num> the analyzer will switch in 10 dB attenuation.

**Note:** This command will accept **MIN** or **MAX** instead of a numeric parameter. See [SCPI Syntax](#) for more information.

---

#### Examples

```
SOUR:POW:ATT 10
source2:power:attenuation maximum
```

**Query Syntax** SOURce<cnum>:POWER<port>:ATTenuation?

**Return Type** Numeric

**Overlapped?** No



**Default** 0

---

### **SOURce<num>:POWER:ATTenuation:AUTO <ON | OFF>**

(Read-Write) Turns automatic attenuation control ON or OFF. Setting an attenuation value (using SOURce:POWER:ATTenuation <num>) sets AUTO **OFF**.

#### **Parameters**

<num> Any existing channel number. If unspecified, value is set to 1.

<port> Port number of the attenuator being set. Choose 1 or 2; If unspecified, value is set to 1.

<ON | OFF> **ON** (or 1) - turns coupling ON. The analyzer automatically selects the appropriate attenuation level to meet the specified power level.

**OFF** (or 0) - turns coupling OFF. Attenuation level must be set using SOURce:POWER:ATTenuation <num>.

#### **Examples**

```
SOUR:POW2:ATT:Auto On
source2:power:
 attentuation:auto off
```

**Query Syntax** SOURce<num>:POWER:ATTenuation:Auto?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

### **SOURce<num>:POWER:CENTer <num>**

(Read-Write) Sets the power sweep center power. Must also set: SENS:SWE:TYPE POWER and SOURce:POWER:SPAN <num>.

#### **Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<num> Center power. Actual achievable leveled power depends on frequency.

#### **Examples**

```
SOUR:POW:CENT -15
source2:power:center -7
```

**Query Syntax** SOURce<num>:POWER:CENTer?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 dBm

---

## SOURce<cnum>:POWER:COUPlE <ON | OFF>

(Read-Write) Turns Port Power Coupling ON or OFF.

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON | OFF> **ON** (or 1) - turns coupling ON. Power level can be set individually for each source port.  
**OFF** (or 0) - turns coupling OFF. The same power level is used for both source ports.

### Examples

```
SOUR:POW:COUP ON
source2:power:couple off
```

**Query Syntax** SOURce<cnum>:POWER:COUPlE?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON

---

## SOURce<cnum>:POWER:DETector <char>

(Read-Write) Sets the source leveling loop as Internal or External.

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<char> **INTernal** - Internal leveling is applied to the source

**EXTernal** - External leveling is applied to the source through a rear-panel connector.  
ONLY provided on 3 GHz, 6 GHz, and 9 GHz PNA models.

### Examples

```
SOUR:POW:DET INT
source2:power:detector external
```

**Query Syntax** SOURce<cnum>:POWER:DETector?

**Return Type** Character

**Overlapped?** No

**Default** INTernal

---

## SOURce<cnum>:POWER<port>[:LEVel][:IMMediate] [:AMPLitude] <num>

(Read-Write) Sets the RF power output level.

**Parameters**

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <port> Port number of the attenuator being set. Choose **1** or **2**; If unspecified, value is set to 1.
- <num> Source power in dBm.

---

**Note:** The range of settable power values depends on the PNA model and if source attenuators are installed. To determine the range of values, perform a query using MAX, then MIN, as an argument. (SOUR:POW:ATT:AUTO must be set to ON) Example: SOURce:POWer? Max

---

Actual achievable leveled power depends on frequency.

**Examples**

```
SOUR:POW1 5DB
source2:power:level
:immediate:amplitude maximum
```

**Query Syntax** SOURce<cnm>:POWer[:LEVel][:IMMediate][:AMPLitude]?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 dBm

---

**SOURce<cnm>:POWer[:LEVel]:SLOPe <num>**

(Read-Write) Sets the RF power slope value.

**Parameters**

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <num> Slope value in db/GHz. Choose any integer between **-2** and **2** (0 is no slope).

**Examples**

```
SOUR:POW:SLOP 2
source2:power:slope -2
```

**Query Syntax** SOURce<cnm>:POWer[:LEVel]:SLOPe?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**SOURce<cnm>:POWer[:LEVel]:SLOPe:STATe <ON | OFF>**

(Read-Write) Turns Power Slope ON or OFF.

**Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<ON|OFF> **ON** (or 1) - turns slope ON.  
**OFF** (or 0) - turns slope OFF.

**Examples** `SOUR:POW:SLOP:STAT ON`  
`source2:power:slope:state off`

**Query Syntax** `SOURce<num>:POWER[:LEVel]:SLOPe:STATe?`

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF

---

**SOURce<num>:POWER:SPAN <num>**

(Read-Write) Sets the power sweep span power. Must also set:

SENS:SWE:TYPE POWER and SOURce:POWER:CENTer <num>.

**Parameters**

<num> Any existing channel number. If unspecified, value is set to 1

<num> Span power. Actual achievable leveled power depends on frequency.

**Examples** `SOUR:POW:SPAN -15`  
`source2:power:span -7`

**Query Syntax** `SOURce<num>:POWER:SPAN?`

**Return Type** Numeric

**Overlapped?** No

**Default** 0 dBm

---

**SOURce<num>:POWER:START <num>**

(Read-Write) Sets the power sweep start power. Must also set SENS:SWE:TYPE POWER and SOURce:POWer:STOP <num>.

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<num> Start power.

---

**Note:** The range of settable power values depends on the PNA model and if source attenuators are installed. To determine the range of values, perform a query using MAX, then MIN, as an argument. (SOUR:POW:ATT:AUTO must be set to ON) Example: SOURce:POWer:STARt? MIN

---

Actual achievable leveled power depends on frequency.

### Examples

```
SOUR:POW:STAR -15
source2:power:start -7
```

**Query Syntax** SOURce<cnum>:POWer:STARt?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 dBm

---

## SOURce<cnum>:POWer:STOP <num>

(Read-Write) Sets the power sweep stop power. Must also set: SENS:SWE:TYPE POWER and SOURce:POWer:STARt <num>.

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<num> Stop power.

---

**Note:** The range of settable power values depends on the PNA model and if source attenuators are installed. To determine the range of values, perform a query using MAX, then MIN, as an argument. (SOUR:POW:ATT:AUTO must be set to ON) Example: SOURce:POWer:STOP? MAX

---

Actual achievable leveled power depends on frequency.

### Examples

```
SOUR:POW:STOP -15
source2:power:stop -7
```

**Query Syntax** SOURce<cnum>:POWer:STOP?

**Return Type** Numeric

**Overlapped?** No


**Default** 0 dBm



## Source:Power:Correction Commands

---

Controls the source power correction features of the analyzer.

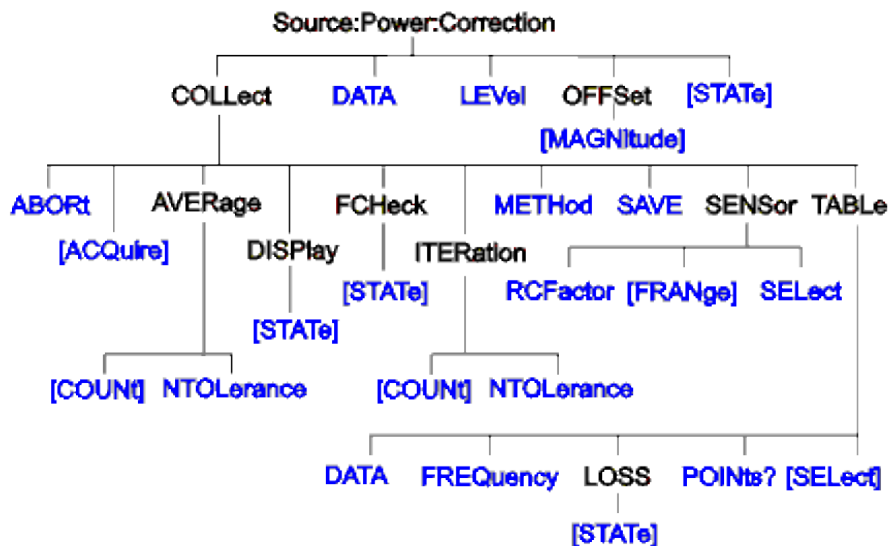

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- See an [example](#) program using these commands.
- See a [template](#) for creating your own Power Meter Driver
- [Learn about Source Cal](#)

---

**Note:** The `SOURce:POWer:CORRection:COLLect:ACQuire` command, used to step the PNA and read a power meter, cannot be sent over the GPIB unless the power meter is connected to a different GPIB interface. See the alternative methods described in the command details.

---

SOURce:POWer:CORRection:COLLect:ABORt

## **SOURce<cnum>:POWER<port>:CORRection:COLLect:ABORT**

(Write-only) Aborts a source power calibration sweep that is in progress.

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.

### Examples

```
SOUR:POW:CORR:COLL:ABOR
source1:power2:correction:collect:abort
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## **SOURce<cnum>:POWER<port>:CORRection:COLLect[:ACQuire] <char>**

(Write-only) Initiates a source power cal acquisition sweep using the power sensor attached to the specified channel (A or B) on the power meter.

**Note:** This command, used to step the PNA and read a power meter, cannot be sent over the GPIB unless the power meter is connected to a different GPIB interface. Use one of the following methods to perform this command or its equivalent:

- Connect the power meter to the PNA using a [USB / GPIB interface](#) (Agilent 82357A).
- SCPI programming of the PNA using a LAN Client interface ([see example](#))
- Send SCPI commands through the COM interface using the [SCPI String Parser](#) object.
- Directly control the Power Meter and PNA to step frequency; then acquire and store the Power reading. ([see example](#))

### Parameters

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.
- <char> Choose from:

**ASENSor** - Sensor on power meter channel A

**BSENSor** - Sensor on power meter channel B

### Examples

```
SOUR:POW:CORR:COLL ASENS
source1:power2:correction:collect:acquire bsensor
```

**Query Syntax** Not Applicable



**Overlapped?** No

**Default** Not Applicable

---

### **SOURce<cnum>:POWER<port>:CORRection:COLLect:AVERAge[:COUNT] <num>**

(Read-Write) Specifies the maximum number of power readings that are taken at each stimulus point to allow for power meter settling. Each reading is averaged with the previous readings at that stimulus point. When this average meets the Average:NTOLerance value or this number of readings has been made, the average is returned as the valid reading.

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<port> Port number to correct for source power. If unspecified, value is set to 1.

<num> Maximum number of readings to make to allow for settling. Choose any number between 3 and 25.

#### **Examples**

```
SOUR:POW:CORR:COLL:AVER 2
source1:power2:correction:collect:average:count 3
```

**Query Syntax** SOURce:POWER:CORRection:COLLect:AVERAge[:COUNT]?

**Return Type** Numeric

**Overlapped?** No

**Default** 3

---

### **SOURce<cnum>:POWER<port>:CORRection:COLLect:AVERAge:NTOLerance <num>**

(Read-Write) Each power reading is averaged with the previous readings at each stimulus point. When the average meets this nominal tolerance value or the max number of readings has been made, the average is returned as the valid reading.

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<port> Port number to correct for source power. If unspecified, value is set to 1.

<num> Power meter settling tolerance value in dB. Choose any number between 0 and 5.

#### **Examples**

```
SOUR:POW:CORR:COLL:AVER:NTOL .05
source1:power2:correction:collect:average:ntolerance .003
```

**Query Syntax** SOURce:POWER:CORRection:COLLect:AVERAge:NTOLerance?

**Return Type** Numeric

**Overlapped?** No

**Default** .050 dBm

---

### **SOURce<cnum>:POWER:CORRection:COLLect:DISPlay[:STATe] <ON | OFF>**

(Read-Write) Enables and disables the display of power readings on the PNA screen. Send this command BEFORE you begin a source power cal acquisition. After the source power cal data is acquired, this setting is reset to ON.

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON|OFF> **ON (1)** Source power calibration dialog box is shown on the PNA screen. Power meter readings are plotted against the Tolerance value as limit lines.

**OFF (0)** - Source power calibration dialog box is NOT shown on the PNA screen.

#### **Examples**

```
SOUR:POW:CORR:COLL:DISP ON
source1:power2:correction:collect:display:state off
```

**Query Syntax** SOURce:POWER:CORRection:COLLect:DISPlay[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** ON (1)

---

### **SOURce<cnum>:POWER:CORRection:COLLect:FCHeck[:STATe] <ON | OFF>**

(Read-Write) Enables and disables frequency checking of source power cal acquisition sweeps. ONLY use when you have more than one power sensor.

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON|OFF> **ON (1)** turns source power cal frequency checking ON. A requested acquisition will only succeed for those frequency points which fall within a frequency range specified for the power sensor being used. An acquisition will pause in mid-sweep if the frequency is about to exceed the maximum frequency limit specified for that sensor. When the sweep is paused in this manner, a sensor connected to the other channel input of the power meter can be connected to the measurement port in place of the previous sensor, and used to complete the sweep. However, the maximum frequency specified for the second sensor would need to be sufficient for the sweep to complete. Frequency limits are specified using the SOUR:POW:CORR:COLL:SEN command.

**OFF (0)** - turns source power cal frequency checking OFF. An acquisition will use just one power sensor for the entire sweep, regardless of frequency.

**Examples** `SOUR:POW:CORR:COLL:FCH ON`  
`source1:power2:correction:collect:fcheck:state off`

**Query Syntax** SOURce:POWer:CORRection:COLLect:FCHeck[:STATe]?

**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF (0)

---

### **SOURce<cnum>:POWER<port>:CORRection:COLLect:ITERation[:COUNT] <num>**

(Read-Write) Sets the maximum number of readings to take at each data point for iterating the source power. Power readings will continue to be made, and source power adjusted, until a reading is within the iteration tolerance value or this max number of readings has been met. The last value to be read is the valid reading for that data point.

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<port> Port number to correct for source power. If unspecified, value is set to 1.

<num> Maximum number of readings. Choose any number between 1 and 100.

**Examples** `SOUR:POW:CORR:COLL:ITER 2`  
`source1:power2:correction:collect:iteration 3`

**Query Syntax** SOURce:POWer:CORRection:COLLect:ITERation[:COUNT]?

**Return Type** Numeric

**Overlapped?** No

**Default** 1

---

### **SOURce<cnum>:POWER<port>:CORRection:COLLect:ITERation:NTOLerance <num>**

(Read-Write) Sets the maximum desired deviation from the sum of the test port power and the offset value. Power readings will continue to be made, and source power adjusted, until a reading is within this tolerance value or the max number of readings has been met. The last value to be read is the valid reading for that data point.

**Parameters**

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.
- <num> Tolerance value in dBm. Choose any number between 0 and 5

**Examples**

```
SOUR:POW:CORR:COLL:ITER:NTOL .005
source1:power2:correction:collect:iteration:ntolerance .1
```

**Query Syntax** SOURce:POWer:CORRection:COLLect:ITERation:NTOLerance?

**Return Type** Numeric

**Overlapped?** No

**Default** .05

---

**SOURce<cnm>:POWer<port>:CORRection:COLLect:METhod <char>**

(Read-Write) Selects the calibration method to be used for the source power cal acquisition.

**Parameters**

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.
- <char> Choose from:
  - NONE** - No Cal method
  - PMETer** - Power Meter is used for all readings. (same as "fast iteration" box not checked on dialog box)
  - PMReceiver** - Power meter for the first iteration; then use the reference receiver for remaining readings if necessary (same as "fast iteration" box checked on dialog box)

**Examples**

```
SOUR:POW:CORR:COLL:METH PMET
source1:power2:correction:collect:method pmreceiver
```

**Query Syntax** SOURce:POWer:CORRection:COLLect:METhod?

**Return Type** Character

**Overlapped?** No

**Default** NONE

---

## **SOURce<cnum>:POWER<port>:CORRection:COLLect:SAVE**

(Write-only) Applies the array of correction values after a source power calibration sweep has completed. The source power correction will then be active on the specified source port for channel <cnum>. This command does NOT save the correction values. To save correction values, save an instrument / calibration state (\*.cst file) after performing a source power cal.

### **Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.

### **Examples**

```
SOUR:POW:CORR:COLL:SAVE
source1:power2:correction:collect:save
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## **SOURce<cnum>:POWER:CORRection:COLLect:<pmChan>SENSor[:FRANge] <num1>,<num2>**

(Read-Write) Specifies the frequency range over which the power sensors connected to the specified channels (A and B) of the power meter can be used (minimum frequency, maximum frequency). If the power meter has only a single channel, that channel is considered channel A.

### **Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <pmChan> Power Meter channel. Choose from:  
A - Channel A  
B - Channel B
- <num1> Minimum frequency for the sensor. If a frequency unit is not specified, Hz is assumed. No limits are placed on this value.
- <num2> Maximum frequency for the sensor. If a frequency unit is not specified, Hz is assumed. No limits are placed on this value.

### **Examples**

```
SOUR:POW:CORR:COLL:ASEN 100E3, 3E9
source1:power2:correction:collect:bsensor:frange 10 MHz, 18 GHz
```

---

|                     |                                                                                                        |
|---------------------|--------------------------------------------------------------------------------------------------------|
| <b>Query Syntax</b> | SOURce:POWer:CORRection:COLLect:ASENsor[:FRANge]?<br>SOURce:POWer:CORRection:COLLect:BSENsor[:FRANge]? |
| <b>Return Type</b>  | Numeric                                                                                                |
| <b>Overlapped?</b>  | No                                                                                                     |
| <b>Default</b>      | 0,0                                                                                                    |

---

### **SOURce<cnum>:POWer:CORRection:COLLect:<pmChan>SENsor:RCFactor <num>**

(Read-Write) ) Specifies the reference cal factor for the power sensor connected to channel A or B of the power meter. If the power meter has only a single channel, that channel is considered channel A.

**Note:** If the sensor connected to the specified channel of the power meter contains cal factors in EPROM (such as the Agilent E-series power sensors), those will be the cal factors used during the calibration sweep. The reference cal factor value associated with this command, and any cal factors entered into the PNA for that sensor channel, will not be used.

---

#### **Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <pmChan> Power Meter channel. Choose from:
  - A** - Channel A
  - B** - Channel B
- <num> Reference cal factor in percent. Choose any number between 1 and 150.

#### **Examples**

```
SOUR:POW:CORR:COLL:ASEN:RCF 98.7
source1:power2:correction:collect:bsensor:rcfactor 105
```

|                     |                                                                                                        |
|---------------------|--------------------------------------------------------------------------------------------------------|
| <b>Query Syntax</b> | SOURce:POWer:CORRection:COLLect:ASENsor:RCFactor?<br>SOURce:POWer:CORRection:COLLect:BSENsor:RCFactor? |
| <b>Return Type</b>  | Numeric                                                                                                |
| <b>Overlapped?</b>  | No                                                                                                     |
| <b>Default</b>      | 100                                                                                                    |

---

### **SOURce<cnum>:POWer:CORRection:COLLect:<pmChan>SENsor:SElect**

(Read-Write) Sets and returns the power sensor channel (A or B) to be used. This performs the same function as the **Use this sensor only** checkbox in the Power Sensor Settings dialog.

---

**Note:** This write portion of this command is only necessary when performing an SMC calibration.

---

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<pmChan> Power Meter channel. Choose from:

A - Channel A

B - Channel B

#### Examples

```
SOUR:POW:CORR:COLL:<pmChan>SEN:SEL 'Write
source1:power2:correction:collect:bsensor:select? 1e9 'Read
```

#### Query Syntax

SOURce:POWer:CORRection:COLLect:ASENsor:SELEct? <Frequency>

SOURce:POWer:CORRection:COLLect:BSEnSor:SELEct? <Frequency>

Returns a boolean 1 or 0 (true or false) indicating whether the sensor is to be used at the specified frequency.

If frequency checking is OFF, then the <Frequency> parameter is ignored. The query returns if the sensor is selected for ALL frequencies.

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

## SOURce<num>:POWer:CORRection:COLLect:TABLE:DATA <data>

(Read-Write) Read or write data into the selected table. If the selected table is a power sensor table, the data is interpreted as cal factors in units of percent. If the loss table is selected, the data is interpreted as loss in units of dB.

#### Parameters

<num> Any existing channel number. If unspecified, value is set to 1

<data> Data to write into the selected table.

#### Examples

```
SOURce:POWer:CORRection:COLLect:TABLE:DATA 0.12, 0.34, 0.56
```

#### Query Syntax

SOURce<num>:POWer:CORRection:COLLect:TABLE:DATA?

If the selected table is currently empty, no data is returned.

**Return Type** Numeric - one number per table segment

**Overlapped?** No

**Default** Not Applicable

---

### **SOURce<cnum>:POWER:CORRection:COLLect:TABLE:FREQUency <data>**

(Read-Write) Read or write frequency values for the selected table (cal factor table for a power sensor, or the loss compensation table).

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<data> Frequency data to write into the selected table.

#### **Examples**

```
SOURce:POWER:CORRection:COLLect:TABLE:FREQUency 10E6, 1.5E9, 9E9
```

#### **Query Syntax**

SOURce<cnum>:POWER:CORRection:COLLect:TABLE:FREQUency?

If the selected table is currently empty, no data is returned.

#### **Return Type**

Numeric - one number per table segment

#### **Overlapped?**

No

#### **Default**

Not Applicable

---

### **SOURce<cnum>:POWER:CORRection:COLLect:TABLE:LOSS[:STATE] <ON | OFF>**

(Read-Write) Indicates whether or not to adjust the power readings using the values in the loss table during a source power cal sweep.

#### **Parameters**

<cnum> Any existing channel number. If unspecified, value is set to 1

<ON|OFF> **ON (or 1)** - turns use of the loss table ON.

**OFF (or 0)** - turns use of the loss table OFF.

#### **Examples**

```
SOUR:POW:CORR:COLL:TABL:LOSS ON
source1:power2:correction:collect:table:loss:state off
```

#### **Query Syntax**

SOURce:POWER:CORRection:COLLect:TABLE:LOSS[:STATE]?

#### **Return Type**

Boolean (1 = ON, 0 = OFF)

#### **Overlapped?**

No

#### **Default**

OFF (0)

---



## SOURce<cnum>:POWER:CORRection:COLLect:TABLE:POINts?

(Read-only) Returns the number of segments that are currently in the selected table.

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

### Examples

```
SOUR:POW:CORR:COLL:TABL:POIN?
source1:power2:correction:collect:table:points?
```

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## SOURce<cnum>:POWER:CORRection:COLLect:TABLE[:SElect] <char>

(Read-Write) Selects which table (cal factor table for a power sensor, or the loss compensation table) you want to write to or read from. Read or write using SOURce:POWER:CORRection:COLLect:TABLE:FREQuency and SOURce:POWER:CORRection:COLLect:TABLE:DATA

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1

<char> Choose from:

**NONE** - No table selected

**ASENSOR** - Cal Factor table for Power Sensor A

**BSENSOR** - Cal Factor table for Power Sensor B

**LOSS** - Loss compensation table

### Examples

```
SOUR:POW:CORR:COLL:TABL ASEN
source1:power2:correction:collect:table:select bsensor
```

**Query Syntax** SOURce:POWER:CORRection:COLLect:TABLE[:SElect]?

**Return Type** Character

**Overlapped?** No

**Default** NONE

---

## SOURce<cnum>:POWER<port>:CORRection:DATA <data>

(Read-Write) Writes and reads source power calibration data.

When querying source power calibration data, if no source power cal data exists for the specified channel and source port, no data is returned.

If a change in the instrument state causes interpolation and/or extrapolation of the source power cal, the correction data associated with this command correspond to the new instrument state (interpolated and/or extrapolated data).

If the channel is sweeping the source backwards, then the first data point is the highest frequency value; the last data point is the lowest. Use the SENS:X:VALues? command to return the X-axis values in the displayed order.

### Parameters

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.
- <data> Correction Data

**Examples** `SOURce1:POWer2:CORRection:DATA 0.12, -0.34, 0.56`

**Query Syntax** `SOURce<cnm>:POWer<port>:CORRection:DATA?`

**Return Type** Depends on FORMat:DATA command

**Overlapped?** No

**Default** Not Applicable

---

## SOURce<cnm>:POWer<port>:CORRection:LEVel <num>

(Read-Write) Specifies the power level that is expected at the desired reference plane (DUT input or output). This is not used for segment sweep with independent power levels or power sweeps.

**Note:** Although this command still works, it is recommended that you specify cal power by setting the test port power and offset value.

### Parameters

- <cnm> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.
- <num> Cal power level in dBm. Because this could potentially be at the output of a device-under-test, no limits are placed on this value here. It is realistically limited by the specifications of the device (power sensor) that will be used for measuring the power. The power delivered to the PNA receiver must never exceed PNA specifications for the receiver!

**Examples** `SOUR:POW:CORR:LEV 10`  
`source1:power2:correction:level 0 dbm`

**Query Syntax** `SOURce:POWer:CORRection:LEVel?`

**Return Type** Numeric

**Overlapped?** No

**Default** 0 dBm

---

### **SOURce<cnum>:POWER<port>:CORRection:OFFSet[:MAGNitude] <num>**

(Read-Write) Sets or returns a power level offset from the PNA test port power. This can be a gain or loss value (in dB) to account for components you connect between the source and the reference plane of your measurement. For example, specify 10 dB to account for a 10 dB amplifier at the input of your DUT.

Cal power is the sum of the test port power setting and this offset value. Following the calibration, the PNA power readouts are adjusted to the cal power.

#### **Parameters**

- <cnum> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.
- <num> Gain or loss value in dB. Choose a value between -200 and 200

#### **Examples**

```
SOUR:POW:CORR:OFFS 10
source1:power2:correction:offset:magnitude -3
```

**Query Syntax** SOURce:POWER:CORRection:OFFSet[:MAGNitude]?

**Return Type** Numeric

**Overlapped?** No

**Default** 0 dB

---

### **SOURce<cnum>:POWER<port>:CORRection[:STATe] <ON|OFF>**

(Read-Write) Enables and disables source power correction for the specified port on the specified channel.

**Parameters**

- <num> Any existing channel number. If unspecified, value is set to 1
- <port> Port number to correct for source power. If unspecified, value is set to 1.
- <ON|OFF> ON (or 1) turns source power correction ON.  
OFF (or 0) - turns source power correction OFF.

**Examples**

```
SOUR:POW:CORR ON
source1:power2:correction:state off
```

**Query Syntax** SOURce:POWer:CORRection[:STATe]?


**Return Type** Boolean (1 = ON, 0 = OFF)

**Overlapped?** No

**Default** OFF (0)

## Status Register Commands

The status registers enable you to query the state of selected events that occur in the analyzer.

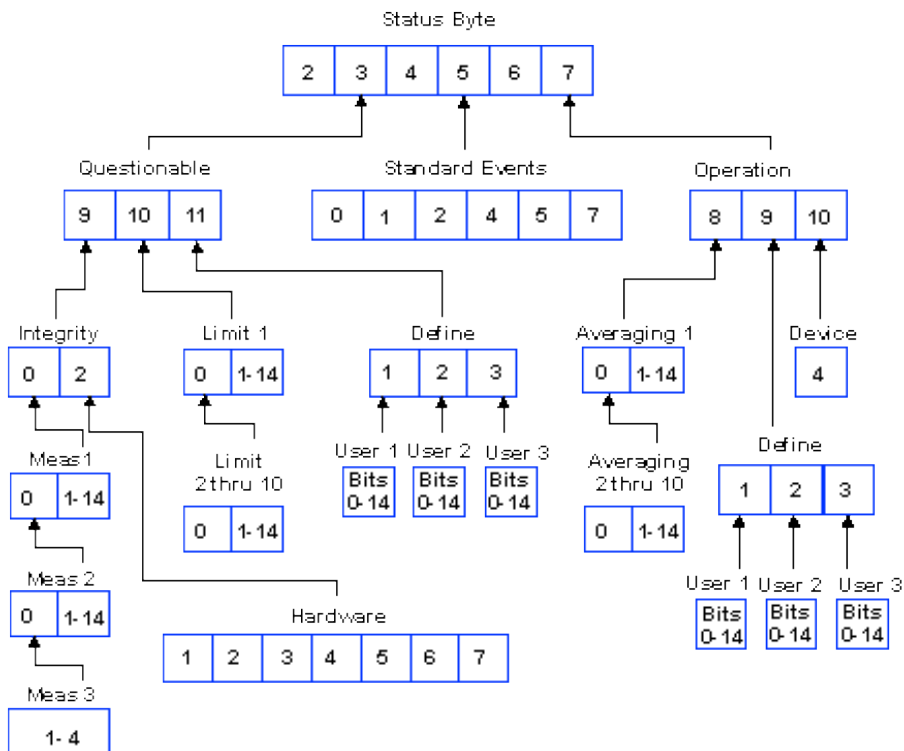

**Note:** This documentation requires familiarity with the "Standard Status Data Structure - Register Model" as defined in IEEE Std 488.2-1992.

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Status Registers](#)

**Note:** Any bit not shown in the registers is not used but may be reserved for future use.

## Status Byte Register

Summarizes the states of the other registers and monitors the PNA output queue. It also generates **service requests**. The Enable register is called the Service Request Enable Register.

| Commands   | Description                                                                                                                                                                                                                       |
|------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| *CLS       | Clears ALL "event" registers and the SCPI Error / Event queue. The corresponding ENABLE registers are unaffected.                                                                                                                 |
| *STB?      | Reads the value of the analyzer's status byte. The byte remains after being read.                                                                                                                                                 |
| *SRE?      | Reads the current state of the Service Request <b>Enable</b> Register.                                                                                                                                                            |
| *SRE <num> | Sets bits in the Service Request <b>Enable</b> register. The current setting of the SRE register is stored in non-volatile memory. Use *SRE 0 to clear the enable.<br><br><num> Combined value of the weights for bits to be set. |

| Bit | Weight | Description                       | Bit is set to 1 when the following conditions exist:                                                                                                                |
|-----|--------|-----------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 2   | 4      | Error / Event queue Summary (EAV) | the Error / Event queue is not empty. To read the error message, use <u>SYST:ERR?</u>                                                                               |
| 3   | 8      | Questionable Register Summary     | any enabled bit in the <b>questionable</b> event status register is set to 1                                                                                        |
| 4   | 16     | Message Available                 | the output queue is not empty                                                                                                                                       |
| 5   | 32     | Standard Event Register Summary   | any enabled bit in the <b>standard</b> event status register is set to 1                                                                                            |
| 6   | 64     | Request Service                   | any of the other bits in the status byte register is set to 1 (used to alert the controller of a service request within the analyzer). This bit cannot be disabled. |
| 7   | 128    | Operation Register Summary        | any enabled bit in the standard <b>operation</b> event status register is set to 1                                                                                  |

## STATus:QUEStionable:<keyword>

Summarizes conditions that monitor the quality of measurement data.

**<keyword>**    **Example**

:CONDition?    **STAT:QUES:COND?**

:ENABle <bits>    **STAT:QUES:ENAB 1024**

[:EVENT]?    **STAT:QUES?**

:NTRansition  
<bits>    **STAT:QUES:NTR 1024**

:PTRansition  
<bits>    **STAT:QUES:PTR 0**

| Bit | Weight | Description              | Bit is set to 1 when the following conditions exist:               |
|-----|--------|--------------------------|--------------------------------------------------------------------|
| 9   | 512    | Integrity Reg summary    | any enabled bit in the <b>Integrity</b> event register is set to 1 |
| 10  | 1024   | Limit Registers summary  | any enabled bit in the <b>Limit</b> event registers is set to 1    |
| 11  | 2048   | Define Registers summary | any enabled bit in the <b>Define</b> event registers is set to 1   |

## STATus:QUEStionable:INTegrity <keyword>

Summarizes conditions in the Measurement Integrity register.

**<keyword>**    **Example**

:CONDition?    **STAT:QUES:INT:COND?**

:ENABle <bits>    **STAT:QUES:INT:ENAB 1024**

[:EVENT]?    **STAT:QUES:INT?**

:NTRansition <bits>    **STAT:QUES:INT:NTR 1024**

:PTRansition <bits>    **STAT:QUES:INT:PTR 0**

| Bit | Weight | Description         | Bit is set to 1 when the following conditions exist:                   |
|-----|--------|---------------------|------------------------------------------------------------------------|
| 0   | 1      | Measurement Summary | any bit in the <b>Measurement Integrity</b> event register is set to 1 |
| 2   | 2      | Hardware Summary    | any bit in the <b>Hardware</b> event register is set to 1              |

## STATus:QUEStionable:INTegrity:HARDware<keyword>

Monitors the status of hardware failures.

| <keyword>           | Example                      |
|---------------------|------------------------------|
| :CONDition?         | STAT:QUES:INT:HARD:COND?     |
| :ENABle <bits>      | STAT:QUES:INT:HARD:ENAB 1024 |
| [:EVENT]?           | STAT:QUES:INT:HARD?          |
| :NTRansition <bits> | STAT:QUES:INT:HARD:NTR 1024  |
| :PTRansition <bits> | STAT:QUES:INT:HARD:PTR 0     |

| Bit | Weight | Description     | Bit is set to 1 when the following conditions exist:                                                                                                                        |
|-----|--------|-----------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1   | 2      | Phase Unlock    | the source has lost phaselock, possibly caused by a reference channel open or a hardware failure.                                                                           |
| 2   | 4      | Unleveled       | the source power is unleveled. This could be caused by a source set for more power than it can deliver at the tuned frequency. Or it could be caused by a hardware failure. |
| 3   | 8      | Overpower       | too much power is detected at the input. This is from either using an amplifier, or a hardware failure.                                                                     |
| 4   | 16     | EE Write Failed | an attempted write to the EEPROM has failed, possibly caused by a hardware failure.                                                                                         |
| 5   | 32     | YIG Cal Failed  | the analyzer was unable to calibrate the YIG. Either the phaselock has been lost or there has been a hardware failure.                                                      |
| 6   | 64     | Ramp Cal Failed | the analyzer was unable to calibrate the analog ramp generator due to a possible hardware failure.                                                                          |
| 7   | 128    | OverTemp        | the source temperature sensor exceeds the limit. It could result from restricted airflow or a broken fan                                                                    |



**STATus:QUEStionable:INTEgrity:MEASurement<n> <keyword>**

Monitors the lag between changing a channel setting and when the data is ready to query.

When you change the channel state (start/stop freq, bandwidth, and so forth), then the questionable bit for that channel is set. This indicates that your desired channel state does not yet match the data you would get if querying a data trace. When the next sweep is complete (without aborting in the middle), and the data trace matches the channel state that produced it, the bit is cleared for that channel.

<n> Measurement register number. Choose from 1 to 3

**<keyword> Example**

|                     |                               |
|---------------------|-------------------------------|
| :CONDition?         | STAT:QUES:INT:MEAS1:COND?     |
| :ENABle <bits>      | STAT:QUES:INT:MEAS2:ENAB 1024 |
| [:EVENT]?           | STAT:QUES:INT:MEAS3?          |
| :NTRansition <bits> | STAT:QUES:INT:MEAS2:NTR 1024  |
| :PTRansition <bits> | STAT:QUES:INT:MEAS1:PTR 0     |

|     |        | Measurement Register <n> |                         |    |                                                                                              |
|-----|--------|--------------------------|-------------------------|----|----------------------------------------------------------------------------------------------|
| Bit | Weight | 1                        | 2                       | 3  | Bit is set to 1 when the following conditions exist:                                         |
| 0   | 1      | 1                        | Summary from Meas Reg 3 |    | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 1   | 2      | 2                        | 15                      | 29 | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 2   | 4      | 3                        | 16                      | 30 | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 3   | 8      | 4                        | 17                      | 31 | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 4   | 16     | 5                        | 18                      | 32 | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 5   | 32     | 6                        | 19                      |    | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 6   | 64     | 7                        | 20                      |    | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 7   | 128    | 8                        | 21                      |    | a setting change on this channel has occurred and the data does not yet reflect that change. |

|    |       |                         |    |  |                                                                                              |
|----|-------|-------------------------|----|--|----------------------------------------------------------------------------------------------|
| 8  | 256   | 9                       | 22 |  | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 9  | 512   | 10                      | 23 |  | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 10 | 1024  | 11                      | 24 |  | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 11 | 2048  | 12                      | 25 |  | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 12 | 4096  | 13                      | 26 |  | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 13 | 8192  | 14                      | 27 |  | a setting change on this channel has occurred and the data does not yet reflect that change. |
| 14 | 16384 | Summary from Meas Reg 2 | 28 |  | a setting change on this channel has occurred and the data does not yet reflect that change. |

### STATus:QUESTIONable:LIMit<n> <keyword>

Monitors and summarizes the status of limit line failures. When a trace fails, the representative bit is set to 1.

Bit 0 is used to summarize failures in the registers that follow. For example, Limit Register 3, bit 0, summarizes the failures from registers 4 through 10.

All enable bits are set to 1 by default.

To find the measurement number, use Calc:Par:Mnum

<n> Limit register: Choose from 1 to 10.

**<keyword> Example**

:CONDition? STAT:QUES:LIM4:COND?

:ENABLE <bits> STAT:QUES:LIM1:ENAB 1024

[:EVENT]? STAT:QUES:LIM3?

:NTRansition <bits> STAT:QUES:LIM2:NTR 1024

:NTRansition? STAT:QUES:LIM1:NTR?

:PTRansition <bits> STAT:QUES:LIM5:PTR 0

:PTRansition? STAT:QUES:LIM1:PTR?

|     |        | Limit Register <n>   |      |      |      |      |      |      |      |     |     |                                                      |
|-----|--------|----------------------|------|------|------|------|------|------|------|-----|-----|------------------------------------------------------|
| Bit | Weight | 1                    | 2    | 3    | 4    | 5    | 6    | 7    | 8    | 9   | 10  | Bit is set to 1 when the following conditions exist: |
| 0   | 1      | 2-10                 | 3-10 | 4-10 | 5-10 | 6-10 | 7-10 | 8-10 | 9,10 | 10  |     | Summary - Any point from these registers fails       |
|     |        | <b>Trace Numbers</b> |      |      |      |      |      |      |      |     |     |                                                      |
| 1   | 2      | 1                    | 15   | 29   | 43   | 57   | 71   | 85   | 99   | 113 | 127 | any point on trace fails the limit test              |
| 2   | 4      | 2                    | 16   | 30   | 44   | 58   | 72   | 86   | 100  | 114 | 128 | any point on trace fails the limit test              |
| 3   | 8      | 3                    | 17   | 31   | 45   | 59   | 73   | 87   | 101  | 115 |     | any point on trace fails the limit test              |
| 4   | 16     | 4                    | 18   | 32   | 46   | 60   | 74   | 88   | 102  | 116 |     | any point on trace fails the limit test              |
| 5   | 32     | 5                    | 19   | 33   | 47   | 61   | 75   | 89   | 103  | 117 |     | any point on trace fails the limit test              |
| 6   | 64     | 6                    | 20   | 34   | 48   | 62   | 76   | 90   | 104  | 118 |     | any point on trace fails the limit test              |
| 7   | 128    | 7                    | 21   | 35   | 49   | 63   | 77   | 91   | 105  | 119 |     | any point on trace fails the limit test              |
| 8   | 256    | 8                    | 22   | 36   | 50   | 64   | 78   | 92   | 106  | 120 |     | any point on trace fails the limit test              |
| 9   | 512    | 9                    | 23   | 37   | 51   | 65   | 79   | 93   | 107  | 121 |     | any point on trace fails the limit test              |
| 10  | 1024   | 10                   | 24   | 38   | 52   | 66   | 80   | 94   | 108  | 122 |     | any point on trace fails the limit test              |
| 11  | 2048   | 11                   | 25   | 39   | 53   | 67   | 81   | 95   | 109  | 123 |     | any point on trace fails the limit test              |
| 12  | 4096   | 12                   | 26   | 40   | 54   | 68   | 82   | 96   | 110  | 124 |     | any point on trace fails the limit test              |
| 13  | 8192   | 13                   | 27   | 41   | 55   | 69   | 83   | 97   | 111  | 125 |     | any point on trace fails the limit test              |
| 14  | 16384  | 14                   | 28   | 42   | 56   | 70   | 84   | 98   | 112  | 126 |     | any point on trace fails the limit test              |

## STATus:QUEStionable:DEFine<keyword>

Summarizes conditions in the Questionable:Define:User<1|2|3> event registers.

| <keyword>           | Example                 |
|---------------------|-------------------------|
| :CONDition?         | STAT:QUES:DEF:COND?     |
| :ENABle <bits>      | STAT:QUES:DEF:ENAB 1024 |
| [:EVENT]?           | STAT:QUES:DEF?          |
| :NTRansition <bits> | STAT:QUES:DEF:NTR 1024  |
| :PTRansition <bits> | STAT:QUES:DEF:PTR 0     |

| Bit | Weight | Description | Bit is set to 1 when the following conditions exist:   |
|-----|--------|-------------|--------------------------------------------------------|
| 1   | 2      | USER1       | any bit in the <b>USER1</b> event register is set to 1 |
| 2   | 4      | USER2       | any bit in the <b>USER2</b> event register is set to 1 |
| 3   | 8      | USER3       | any bit in the <b>USER3</b> event register is set to 1 |

## STATus:QUEStionable:DEFine:USER<1|2|3><keyword>

Monitors conditions that you define and map in any of the three QUES:DEF:USER event registers.

| <keyword>          | Example                                                                               |
|--------------------|---------------------------------------------------------------------------------------|
| :ENABle <bits>     | STAT:QUES:DEF:USER1:ENABle 1024                                                       |
| [:EVENT]?          | STAT:QUES:DEF:USER1?                                                                  |
| :MAP <bit>,<error> | STAT:QUES:DEF:USER1:MAP 0,-113 'when error -113 occurs, bit 0 in USER1 will set to 1. |

| Bit | Weight | Description | Bit is set to 1 when the following conditions exist: |
|-----|--------|-------------|------------------------------------------------------|
| 0   | 1      | for user    | user defined                                         |
| 1   | 2      | for user    | user defined                                         |
| 2   | 4      | for user    | user defined                                         |
| 3   | 8      | for user    | user defined                                         |
| 4   | 16     | for user    | user defined                                         |
| 5   | 32     | for user    | user defined                                         |
| 6   | 64     | for user    | user defined                                         |
| 7   | 128    | for user    | user defined                                         |
| 8   | 256    | for user    | user defined                                         |
| 9   | 512    | for user    | user defined                                         |
| 10  | 1024   | for user    | user defined                                         |
| 11  | 2048   | for user    | user defined                                         |
| 12  | 4096   | for user    | user defined                                         |
| 13  | 8192   | for user    | user defined                                         |
| 14  | 16384  | for user    | user defined                                         |

## Standard Event Status Register

Monitors "standard" events that occur in the analyzer. This register can only be cleared by:

- a Clear Command (\*CLS).
- reading the Standard Enable Status Register (\*ESE?).
- a power-on transition. The analyzer clears the register and then records any transitions that occur, including setting the Power On bit (7).

### Commands Description

- \*ESE? Reads the settings of the standard event **ENABLE** register.
- \*ESE **<bits>** Sets bits in the standard event **ENABLE** register. The current setting is saved in non-volatile memory.  
**<bits>** The sum of weighted bits in the register. Use \*ESE 0 to clear the enable register.
- \*ESR? Reads and clears the **EVENT** settings in the Standard Event Status register.
- \*OPC Sets bit 0 when the overlapped command is complete. (see Understanding Command Synchronization / OPC).

\*OPC? Operation complete query - read the Operation Complete bit (0).

| Bit | Weight | Description        | Bit is set to 1 when the following conditions exist:                                                                                                                                                                                                  |
|-----|--------|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 0   | 1      | Operation Complete | the two following events occur <b>in order</b> :<br>1. the *OPC command is sent to the analyzer<br>2. the analyzer completes all pending overlapped commands                                                                                          |
| 1   | NA     | Request Control    | Not Supported - the analyzer application is not configured to control GPIB operation                                                                                                                                                                  |
| 2   | 4      | Query Error        | a query error is detected indicating:<br>- an attempt to read data from the output queue when no data was present <b>OR</b><br>- data in the output queue was lost, as in an overflow                                                                 |
| 4   | 16     | Execution Error    | an execution error is detected indicating:<br>- a <PROGRAM DATA> element was outside the legal range or inconsistent with the operation of the analyzer <b>OR</b><br>- the analyzer could not execute a valid command due to some internal condition  |
| 5   | 32     | Command Error      | a command error is detected indicating that the analyzer received a command that: <ul style="list-style-type: none"> <li>• did not follow proper syntax</li> <li>• was misspelled</li> <li>• was an optional command it does not implement</li> </ul> |
| 7   | 128    | Power ON           | Power to the analyzer has been turned OFF and then ON since the last time this register was read.                                                                                                                                                     |

### STATus:OPERation<keyword>

Summarizes conditions in the Averaging and Operation:Define:User<1|2|3> event registers.

| <keyword>           | Example             |
|---------------------|---------------------|
| :CONDition?         | STAT:OPER:COND?     |
| :ENABle <bits>      | STAT:OPER:ENAB 1024 |
| [:EVENT]?           | STAT:OPER?          |
| :NTRansition <bits> | STAT:OPER:NTR 1024  |
| :PTRansition <bits> | STAT:OPER:PTR 0     |

| Bit | Weight | Description          | Bit is set to 1 when the following conditions exist:                          |
|-----|--------|----------------------|-------------------------------------------------------------------------------|
| 8   | 256    | Averaging summary    | either enabled bit in the <b>Averaging summary</b> event register is set to 1 |
| 9   | 512    | User Defined summary |                                                                               |
| 10  | 1024   | Device summary       | either enabled bit in the <b>Device summary</b> event register is set to 1    |

### STATus:OPERation:AVERaging<n> <keyword>

Monitors and summarizes the status of Averaging on traces 1 to 128. When averaging for a trace is complete, the representative bit is set to 1.

Bit 0 is used to summarize the status in the registers that follow. For example, Average Register, bit 0, summarizes the status from registers 4 through 10.

All enable bits are set to 1 by default.

To find the measurement number, use Calc:Par:Mnum.

<n> Averaging Register. Choose from 1 to 10

#### <keyword> Example

:CONDition? STAT:OPER:AVER1:COND?

:ENABle <bits> STAT:OPER:AVER1:ENAB 1024

[:EVENT]? STAT:OPER:AVER1?

:NTRansition <bits> STAT:OPER:AVER1:NTR 1024

:PTRansition <bits> STAT:OPER:AVER1:PTR 0

|     |        | Averaging Register <n> |      |      |      |      |      |      |      |     |     |                                                           |
|-----|--------|------------------------|------|------|------|------|------|------|------|-----|-----|-----------------------------------------------------------|
| Bit | Weight | 1                      | 2    | 3    | 4    | 5    | 6    | 7    | 8    | 9   | 10  | Bit is set to 1 when the following conditions exist:      |
| 0   | 1      | 2-10                   | 3-10 | 4-10 | 5-10 | 6-10 | 7-10 | 8-10 | 9,10 | 10  |     | Summary - Any enabled bit in these registers is set to 1. |
|     |        | <b>Trace Numbers</b>   |      |      |      |      |      |      |      |     |     |                                                           |
| 1   | 2      | 1                      | 15   | 29   | 43   | 57   | 71   | 85   | 99   | 113 | 127 | Averaging on this trace is complete                       |
| 2   | 4      | 2                      | 16   | 30   | 44   | 58   | 72   | 86   | 100  | 114 | 128 | Averaging on this trace is complete                       |

|    |       |    |    |    |    |    |    |    |     |     |  |                                     |
|----|-------|----|----|----|----|----|----|----|-----|-----|--|-------------------------------------|
| 3  | 8     | 3  | 17 | 31 | 45 | 59 | 73 | 87 | 101 | 115 |  | Averaging on this trace is complete |
| 4  | 16    | 4  | 18 | 32 | 46 | 60 | 74 | 88 | 102 | 116 |  | Averaging on this trace is complete |
| 5  | 32    | 5  | 19 | 33 | 47 | 61 | 75 | 89 | 103 | 117 |  | Averaging on this trace is complete |
| 6  | 64    | 6  | 20 | 34 | 48 | 62 | 76 | 90 | 104 | 118 |  | Averaging on this trace is complete |
| 7  | 128   | 7  | 21 | 35 | 49 | 63 | 77 | 91 | 105 | 119 |  | Averaging on this trace is complete |
| 8  | 256   | 8  | 22 | 36 | 50 | 64 | 78 | 92 | 106 | 120 |  | Averaging on this trace is complete |
| 9  | 512   | 9  | 23 | 37 | 51 | 65 | 79 | 93 | 107 | 121 |  | Averaging on this trace is complete |
| 10 | 1024  | 10 | 24 | 38 | 52 | 66 | 80 | 94 | 108 | 122 |  | Averaging on this trace is complete |
| 11 | 2048  | 11 | 25 | 39 | 53 | 67 | 81 | 95 | 109 | 123 |  | Averaging on this trace is complete |
| 12 | 4096  | 12 | 26 | 40 | 54 | 68 | 82 | 96 | 110 | 124 |  | Averaging on this trace is complete |
| 13 | 8192  | 13 | 27 | 41 | 55 | 69 | 83 | 97 | 111 | 125 |  | Averaging on this trace is complete |
| 14 | 16384 | 14 | 28 | 42 | 56 | 70 | 84 | 98 | 112 | 126 |  | Averaging on this trace is complete |

### STATus:OPERation:DEFine<keyword>

Summarizes conditions in the OPERation:Define:User<1|2|3> event registers.

| <keyword>           | Example               |
|---------------------|-----------------------|
| :CONDition?         | STAT:OPER:DEF:COND?   |
| :ENABle <bits>      | STAT:OPER:DEF:ENAB 12 |
| [:EVENT]?           | STAT:OPER:DEF?        |
| :NTRansition <bits> | STAT:OPER:DEF:NTR 12  |
| :PTRansition <bits> | STAT:OPER:DEF:PTR 0   |



| Bit | Weight | Description | Bit is set to 1 when the following conditions exist:   |
|-----|--------|-------------|--------------------------------------------------------|
| 1   | 2      | USER1       | any bit in the <b>USER1</b> event register is set to 1 |
| 2   | 4      | USER2       | any bit in the <b>USER2</b> event register is set to 1 |
| 3   | 8      | USER3       | any bit in the <b>USER3</b> event register is set to 1 |

### STATus:OPERation:DEFine:USER<1|2|3><keyword>

Monitors conditions that you define and map in any of the three OPER:DEF:USER event registers.

| <u>&lt;keyword&gt;</u> | Example                                                                               |
|------------------------|---------------------------------------------------------------------------------------|
| :ENABLE <bits>         | STAT:OPER:DEF:USER1:ENAB 1024                                                         |
| [:EVENT]?              | STAT:OPER:DEF:USER1?                                                                  |
| :MAP <bit>,<error>     | STAT:OPER:DEF:USER1:MAP 0,-113 'when error -113 occurs, bit 0 in USER1 will set to 1. |

| Bit | Weight | Description | Bit is set to 1 when the following conditions exist: |
|-----|--------|-------------|------------------------------------------------------|
| 0   | 1      | for user    | user defined                                         |
| 1   | 2      | for user    | user defined                                         |
| 2   | 4      | for user    | user defined                                         |
| 3   | 8      | for user    | user defined                                         |
| 4   | 16     | for user    | user defined                                         |
| 5   | 32     | for user    | user defined                                         |
| 6   | 64     | for user    | user defined                                         |
| 7   | 128    | for user    | user defined                                         |
| 8   | 256    | for user    | user defined                                         |
| 9   | 512    | for user    | user defined                                         |
| 10  | 1024   | for user    | user defined                                         |
| 11  | 2048   | for user    | user defined                                         |
| 12  | 4096   | for user    | user defined                                         |
| 13  | 8192   | for user    | user defined                                         |
| 14  | 16384  | for user    | user defined                                         |

---

## STATus:OPERation:DEVIce<keyword>

Summarizes conditions in the OPERation:DEVIce event registers.


| <keyword>           | Example               |
|---------------------|-----------------------|
| :CONDition?         | STAT:OPER:DEV:COND?   |
| :ENABle <bits>      | STAT:OPER:DEV:ENAB 16 |
| [:EVENTi]?          | STAT:OPER:DEV?        |
| :NTRansition <bits> | STAT:OPER:DEV:NTR 16  |
| :PTRansition <bits> | STAT:OPER:DEV:PTR 0   |

---

| Bit | Weight | Description     | Bit is set to 1 when the following conditions exist: |
|-----|--------|-----------------|------------------------------------------------------|
| 0   | 1      | Unused          |                                                      |
| 1   | 2      | Unused          |                                                      |
| 2   | 4      | Unused          |                                                      |
| 3   | 8      | Unused          |                                                      |
| 4   | 16     | Sweep Completed | When sweep is complete                               |
| 5   | 32     | Unused          |                                                      |
| 6   | 64     | Unused          |                                                      |
| 7   | 128    | Unused          |                                                      |
| 8   | 256    | Unused          |                                                      |
| 9   | 512    | Unused          |                                                      |
| 10  | 1024   | Unused          |                                                      |
| 11  | 2048   | Unused          |                                                      |
| 12  | 4096   | Unused          |                                                      |
| 13  | 8192   | Unused          |                                                      |
| 14  | 16384  | Unused          |                                                      |

## System Commands

---

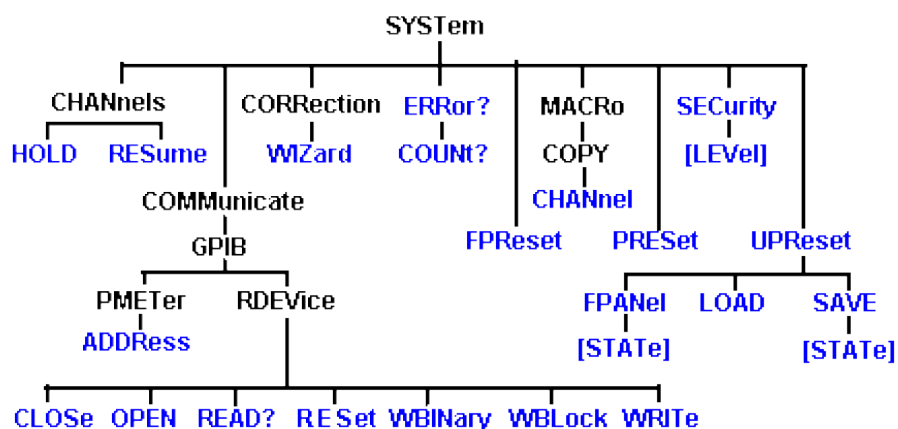

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Preset](#)
- 

### SYSTEM:CHANnels:HOLD

(Write-only) Places all channels in hold mode. To place a single channel in hold mode, use [SENS:SWE:MODE](#).

**Examples** `SYST:CHAN:HOLD`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable



### SYSTEM:CHANnels:RESume

(Write-only) Resumes the trigger mode of all channels that was in effect before sending [SYSTEM:CHANnels:HOLD](#) (must be sent before [SYST:CHAN:RESume](#)).

**Examples** `SYST:CHAN:RES`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**SYSTEM:COMMunicate:GPIB:PMETer:ADDReSS <num>**

(Read-Write) Specifies the GPIB address of the power meter to be used in a source power calibration. When performing a source power cal, the PNA will search VISA interfaces that are configured in the Agilent IO Libraries on the PNA.

**Parameters**

<num> GPIB address of the power meter. Choose any integer between 0 and 30.

**Examples**

```
SYST:COMM:GPIB:PMET:ADDR 13
system:communicate:gpiib:pmeter:address 14
```

**Query Syntax** SYSTem:COMMunicate:GPIB:PMETer:ADDRess?

**Return Type** Numeric

**Overlapped?** No

**Default** 13

---

**SYSTem:COMMunicate:GPIB:RDEvice:CLOSe <ID>**

(Write only) Closes the remote GPIB session. This command should be sent when ending every successful OPEN session.

**Parameters**

<ID> Session identification number that was returned with the OPEN? command.

**Examples**

See an example program

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

**SYSTem:COMMunicate:GPIB:RDEvice:OPEN <bus>, <addr>, <timeout>**

(Read-Write) Initiates a GPIB pass-through session. First send this OPEN command, then send the OPEN query to read the session ID number. An existing GPIB pass-through session remains open after an instrument preset. To learn more about GPIB pass-through capability, see the [example program](#).

#### Parameters

- <bus> Bus ID number. You can find the USB-GPIB adapter bus number by looking at the dialog that appears when the USB-GPIB device is connected.
- <addr> GPIB Address of the device to be controlled
- <timeout> The amount of time (in milliseconds) to wait for a response from the remote device after sending a command. A "timeout" error is displayed after this time has passed without a response.

**Examples** [See an example program](#)

**Query Syntax** SYSTem:COMMunicate:GPIB:RDEvice:OPEN?  
Returns the session identification number that is used when communicating with this device.

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

### SYSTem:COMMunicate:GPIB:RDEvice:READ? <ID>

(Read-only) Returns data from the GPIB pass-through device.

#### Parameters

- <ID> Session identification number that was returned with the [OPEN?](#) command.

**Examples** [See an example program](#)

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

### SYSTem:COMMunicate:GPIB:RDEvice:RESet

(Write-only) Performs the same function as SYST:COMM:GPIB:RDEV:CLOS except that ALL pass-through sessions are closed.

**Examples** `SYST:COMM:GPIB:RDEV:RES`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## **SYSTEM:COMMunicate:GPIB:RDEvice:WBINary <ID>,<data>**

(Write-only) Sends data to a GPIB pass-through device. This command requires a header that specifies the size of the data to be written. The header (described below) is not passed along to the device.

Use this command if too many embedded quotes prevent you from using SYST:COMM:GPIB:RDEV:WRIT.

Use SYST:COMM:GPIB:RDEV:OPEN to open the pass through session.

### **Parameters**

<ID> Session identification number that was returned with the OPEN? command.

<data> Data to be sent to the GPIB pass-through device. Use the following syntax:

`#<num digits><byte count><data bytes><NL><END>`

<num\_digits> specifies how many digits are contained in <byte\_count>

<byte\_count> specifies how many data bytes will follow in <data bytes>

**Examples** `SYSTEM:COMMunicate:GPIB:RDEvice:WBINary 101,#17ABC+XYZ<nl><end>`

# - always sent before data.

1 - specifies that the byte count is one digit (7).

7 - specifies the number of data bytes that will follow, not counting <NL><END>.

ABC+XYZ - Data block

<nl><end> - always sent at the end of block data.

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## **SYSTEM:COMMunicate:GPIB:RDEvice:WBLock <ID>,<data>**

(Write-only) Same as SYSTEM:COMM:GPIB:RDEV:WBIN (above) but the header **IS** passed along to the device. Use this command if too many embedded quotes prevent you from using SYST:COMM:GPIB:RDEV:WRIT.

**Parameters**

<ID> Session identification number that was returned with the OPEN? command.

<data> Data to be sent to the GPIB pass-through device. See previous command.

**Examples** See previous example.

**Query Syntax** Not Applicable

Overlapped? No

Default Not Applicable

---

**SYSTEM:COMMunicate:GPIB:RDEvice:WRITE <ID>,<string>**

(Write-only) Sends ASCII string data to the GPIB pass-through device.

**Parameters**

<ID> Session identification number that was returned with the OPEN? command.

<string> Commands to be sent to the GPIB pass-through device.

**Examples** See an example program

**Query Syntax** Not Applicable

Overlapped? No

Default Not Applicable

---

**SYSTEM:CORRection:WIZard <char>**

(Write-only) Launches either the Calibration Wizard or the Version 2 Calibration Kit File Manager dialog box.

**Parameters**

<char> Choose from:  
MAIN - Launches the Calibration Wizard  
CKIT - Launches the Version 2 Calibration Kit File Manager dialog box.  
Both display on the PNA screen.

**Examples** `SYST:CORR:WIZ MAIN`  
`system:correction:wizard ckit`

**Query Syntax** Not Applicable?

**Overlapped?** No

**Default** Not Applicable

---

**SYSTEM:ERRor?**

(Read-only) Returns the next error in the error queue. Each time the analyzer detects an error, it places a message in the error queue. When the `SYSTEM:ERROR?` query is sent, one message is moved from the error queue to the output queue so it can be read by the controller. Error messages are delivered to the output queue in the order they were received. The error queue is cleared when any of the following conditions occur:

- When the analyzer is switched ON.
- When the `*CLS` command is sent to the analyzer.
- When all of the errors are read.

If the error queue overflows, the last error is replaced with a "Queue Overflow" error. The oldest errors remain in the queue and the most recent error is discarded.

**Examples** `SYST:ERR?`  
`system:error?`

**Overlapped?** No

**Default** Not applicable

---

**SYSTEM:ERRor:COUNT?**

(Read-only) Returns the number of errors in the error queue. Use `SYST:ERR?` to read an error.

**Examples** `SYST:ERR:COUN?`  
`system:error:count?`

**Overlapped?** No

**Default** Not applicable



---

## SYSTem:FPRreset

(Write-only) Performs a standard [Preset](#), then deletes the default trace, measurement, and window. The PNA screen becomes blank.

**Examples** `SYST:FPR  
system:fpreset`

**Overlapped?** No

**Default** Not applicable

---

## SYSTem:MACRo:COpy:CHANnel<cnum>[:TO] <num>

(Write-only) Sets up channel <num> as a copy of channel <cnum>. Learn more about [copy channels](#).

### Parameters

<cnum> Any existing channel number. If unspecified, value is set to 1.

<num> Number of the channel which is to become a copy of channel <cnum>.

**Examples** `SYST:MACR:COpy:CHAN1 2  
system:macro:copy:channel2:to 3`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## SYSTem:PRESet

(Write-only) Deletes all traces, measurements, and windows. In addition, resets the analyzer to factory defined default settings and creates a S11 measurement named "CH1\_S11\_1". For a list of default settings, see [Preset](#).

Regardless of the state of the User Preset Enable checkbox, the SYST:PRESet command will always preset the PNA to the factory preset settings, and [SYST:UPReset](#) will always perform a User Preset.

If the PNA display is disabled with [DISP:ENAB OFF](#) then SYST:PRESet will NOT enable the display.

This command performs the same function as [\\*RST](#).

**Examples** `SYST:PRESet  
system:presSet`

**Overlapped?** No

**Default** Not applicable

---

## SYSTem:SECurity[:LEVel] <char>

(Read-Write) Sets and returns the display of frequency information on the PNA screen and printouts. [Learn more about security level.](#)

### Parameters

<char> Choose from:

**None** - ALL frequency information is displayed

**Low** - NO frequency information is displayed. Frequency information can be redisplayed using the Security Setting dialog box or this command..

**High** - NO frequency information is displayed. Frequency information can be redisplayed ONLY by performing a Preset or recalling an instrument state with None or Low security settings, or using this command.

### Examples

```
SYST:SEC LOW
system:security:level high
```

**Query Syntax** SYSTem:SECurity[:LEVel]?

**Return Type** Character

**Overlapped?** No

**Default** None

---

## SYSTem:UPReset

(Write-only) Performs a User Preset. There must be an active User Preset state file (see [Load](#) and [Save](#)) or an error will be returned. [Learn more about User Preset.](#)

Regardless of the state of the User Preset Enable checkbox, the SYST:PRESet command will always preset the PNA to the factory preset settings, and [SYST:UPReset](#) will always perform a User Preset.

### Examples

```
SYST:UPReset
system:upreset
```

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

---

## SYSTem:UPReset:FPANel[:STATe] <bool>

(Read-Write) 'Checks' and 'clears' the enable box on the [User Preset dialog box](#). This only affects subsequent Presets from the front panel user interface.

Regardless of the state of the User Preset Enable checkbox, the [SYST:PRESet](#) command will always preset the PNA to the factory preset settings, and [SYST:UPReset](#) will always perform a User Preset.

#### Parameters

<bool> Front Panel User Preset State. Choose from:  
0 – User Preset OFF  
1 – User Preset ON

**Examples** `SYST:UPR:FPAN 1`  
`system:upreset:fpanel:state 0`

**Query Syntax** `SYSTem:UPREset:FPANel[:STATe]?`

**Return Type** Boolean

**Overlapped?** No

**Default** 0

### SYSTem:UPReset:LOAD <file>

(Read-Write) Loads an existing instrument state file (.sta or .cst) to be used for User Preset. Subsequent execution of [SYSTem:UPReset](#) will cause the PNA to assume this instrument state.

Regardless of the state of the User Preset Enable checkbox, the [SYST:PRESet](#) command will always preset the PNA to the factory preset settings, and [SYST:UPReset](#) will always perform a User Preset.

[Learn more about User Preset.](#)

#### Parameters

<file> String - Name of the file to be loaded. The default folder "C:\Program Files\Agilent\Network Analyzer\Documents" is used if unspecified. Change the default folder name using [MMEMemory:CDIRectory](#).

**Examples** `SYST:UPR:LOAD '1MHzto20GHzUserPreset.cst'`  
`system:upreset:load 'C:\Documents and Settings\Administrator\My Documents\NewUserPreset.cst'`

**Query Syntax** Not Applicable

**Overlapped?** No

**Default** Not Applicable

## **SYSTem:UPReset:SAVE[:STATe]**

(Write-only) Saves the current instrument settings as UserPreset.sta. Subsequent execution of SYSTem:UPReset will cause the PNA to assume this instrument state.

Regardless of the state of the User Preset Enable checkbox, the SYST:PRESet command will always preset the PNA to the factory preset settings, and SYST:UPReset will always perform a User Preset.

Learn more about User Preset.

|                 |                                                                      |
|-----------------|----------------------------------------------------------------------|
| <b>Examples</b> | <code>SYST:UPR:SAVE</code><br><code>system:upreset:save:state</code> |
|-----------------|----------------------------------------------------------------------|

**Query Syntax** Not Applicable

**Overlapped?** No


**Default** Not Applicable

---

## Trigger Commands

---

Starts or ends a measurement sequence.

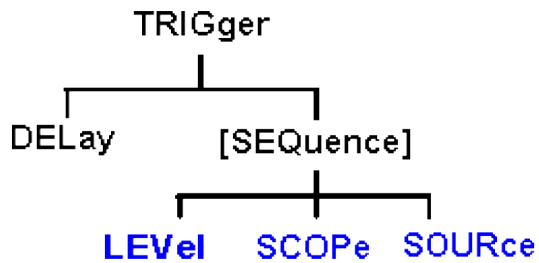

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about Triggering](#)
- 

### TRIGGER:DELAY <num>

(Read-Write) Sets and reads the trigger delay. This delay is only applied while in [External Trigger](#) mode. After an external trigger is applied, the start of the sweep is held off for an amount of time equal to the delay setting plus any inherent latency.

#### Parameters

<num> Delay value in seconds. Choose from 0 to 107.

#### Examples

```
TRIG:DEL .0003
```

```
Sets the trigger delay to 300 microseconds. The sweep will not start until approximately 300 microseconds after an external trigger is applied.
```



**Query Syntax** TRIGGER:DELAY?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### TRIGGER[:SEQUENCE]:LEVEL <char> - OBSOLETE

---

This command is replaced with CONTRol:SIGNal

---

(Read-Write) Triggers either on a **High or Low** level trigger signal. This setting only has an effect when TRIG:SOURce EXTERNAL is selected.

**Parameters**

<char> Choose from:  
**HIGH** - analyzer triggers on TTL **High**  
**LOW** - analyzer triggers on TTL **Low**

**Examples** `TRIG:LEV HIGH`  
`trigger:sequence:level low`

**Query Syntax** TRIGger[:SEQuence]:LEVel?

**Return Type** Character

**Overlapped?** No

**Default** LOW

---

**TRIGger[:SEQuence]:SCOPE <char>**

(Read-Write) Specifies whether triggers are applied to all channels or the current channel.

**Parameters**

<char> Choose from:  
**ALL** - triggers all channels. Also sets SENS:SWEep:TRIG:POINT OFF on **ALL** channels.  
**CURRENT** - trigger only one channel at a time. With each trigger signal, the channel is incremented to the next triggerable channel.

**Examples** `TRIG:SCOP ALL`  
`trigger:sequence:scope current`

**Query Syntax** TRIGger[:SEQuence]:SCOPE?

**Return Type** Character

**Overlapped?** No

**Default** ALL

---

**TRIGger[:SEQuence]:SOURce <char>**

(Read-Write) Sets the source of the sweep trigger signal. This command is a super-set of INITiate:CONTinuous, which can NOT set the source to External. To configure external triggering, see CONTRol:SIGNal.

**Parameters**

<char> Choose from:  
**EXTernal** - external (rear panel) source.  
**IMMEDIATE** - internal source sends continuous trigger signals  
**MANual** - sends one trigger signal when manually triggered from the front panel or INIT:IMM is sent.

**Examples**

```
TRIG:SOUR EXT
trigger:sequence:source immediate
```

**Query Syntax** TRIGger[:SEQuence]:SOURce?

**Return Type** Character

**Overlapped?** No

**Default** IMMEDIATE

## Catalog Measurements using SCPI

---

This Visual Basic Program does the following:

- Catalogs the currently defined measurements, windows, and traces
- Selects a measurement for further definition
- Adds a Title to the window

To run this program, you need:

- An established GPIB interface connection

---

### See Other SCPI Example Programs

---

```
Dim Meas as String
Dim Win as String
Dim Trace as String

'Read the current measurements in Channel 1
GPIB.Write "CALCulate1:PARAmeter:CATalog?"
Meas = GPIB.Read
MsgBox ("Ch1 Measurments: " & Meas)

'Read the current windows
GPIB.Write "DISPlay:CATalog?"
Win = GPIB.Read
MsgBox ("Windows: " & Win)

'Read current traces in window 1
GPIB.Write "DISPlay:WINDow1:CATalog?"
Trace = GPIB.Read
MsgBox ("Traces in Window1: " & Win)
```

---





## Create a Measurement using SCPI

---

This VBScript program creates a new S21 measurement and displays it on the PNA screen.

The SCPI commands in this example are sent over a COM interface using the SCPIStringParser object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as NewMeas.vbs. [Learn how to setup and run the macro.](#)

### [See Other SCPI Example Programs](#)

```
Dim app
Dim scpi
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpiStringParser

' A comment
'Preset the analyzer
scpi.Execute ("SYST:FPRreset")
' Create and turn on window 1
scpi.Execute ("DISPlay:WINDow1:STATE ON")
'Define a measurement name, parameter
scpi.Execute ("CALCulate:PARAmeter:DEFine 'MyMeas',S21")
'Associate ("FEED") the measurement name ('MyMeas') to WINDow (1), and give the new
TRACe a number (1).
scpi.Execute ("DISPlay:WINDow1:TRACe1:FEED 'MyMeas'")
```

## Channels, Windows, and Measurements using SCPI

**SOURce** and most **SENSE** commands act on the **channel** that is specified in the command. Channel 1 is default if not specified.

Most **DISPlay** commands act on the **window and trace** specified in the command. Window1 and Trace1 are default if not specified.

**CALCulate** commands act on the **selected measurement** in the specified channel. Select the measurement for each channel using CALCulate<channel number>:PARAmeter:SELEct <meas name>. You can select one measurement in each channel.

---

The following Visual Basic program does the following:

- Presets the analyzer
- Create 2 windows
- Create 2 Measurements
- Feed the measurements to windows / traces
- Change frequency ranges for channels
- Select both measurements
- Turn marker 1 ON for each measurement

To run this program, you need:

- An established GPIB interface connection

---

### See Other SCPI Example Programs

```
GPIB.Write "SYSTem:PREset"

'Create Measurements
GPIB.Write "CALCulate1:PARAmeter:DEFine 'Meas1',S11"
GPIB.Write "CALCulate2:PARAmeter:DEFine 'Meas2',S21"
↑
' Turn on windows - creates if new
GPIB.Write "DISPlay:WINDow1:STATE ON"
GPIB.Write "DISPlay:WINDow2:STATE ON"

'Associate ("FEED") the measurement name('Meas1') to WINDow(1), and give the new
TRACE a number(1).
GPIB.Write "DISPlay:WINDow1:TRACe1:FEED 'Meas1'"
GPIB.Write "DISPlay:WINDow2:TRACe2:FEED 'Meas2'"

'Change each channel's frequency range
GPIB.Write "SENSE1:FREQuency:SPAN 1e9"
GPIB.Write "SENSE2:FREQuency:SPAN 2e9"

'Select both measurements
GPIB.Write "CALCulate1:PARAmeter:SELEct 'Meas1'"
GPIB.Write "CALCulate2:PARAmeter:SELEct 'Meas2'"
```

```
'Turn marker 1 ON for each measurement
GPIB.Write "CALCulate1:MARKer:STATE ON"
GPIB.Write "CALCulate2:MARKer:STATE ON"
```

## Setup Sweep Parameters using SCPI

---

This Visual Basic program sets up sweep parameters on the Channel 1 measurement. To run this program, you need:

- An established [GPIB interface connection](#)

---

### [See Other SCPI Example Programs](#)

---

```
GPIB.Write "SYSTEM:PRESet"
'Select the measurement
GPIB.Write "CALCulate:PARAMeter:SElect 'CH1_S11_1'"
'Set sweep type to linear
GPIB.Write "SENSE1:SWEep:TYPE LIN"

'Set IF Bandwidth to 700 Hz
GPIB.Write "SENSE1:BANDwidth 700"

'Set Center and Span Freq's to 4 GHz
GPIB.Write "SENSE1:FREQuency:CENTer 4ghz"
GPIB.Write "SENSE1:FREQuency:SPAN 4ghz"

'Set number of points to 801
GPIB.Write "SENSE1:SWEep:POINTs 801"

'Set sweep generation mode to Analog
GPIB.Write "SENSE1:SWEep:GENeration ANAL"

'Set sweep time to Automatic
GPIB.Write "SENSE1:SWEep:TIME:AUTO ON"

'Query the sweep time
GPIB.Write "SENSE1:SWEep:TIME?"
SweepTime = GPIB.Read
```

## Setup the Display using SCPI

---

This Visual Basic program:

- Sets data formatting
- Turns ON the Trace, Title, and Frequency Annotation
- Autoscales the Trace
- Queries Per Division, Reference Level, and Reference Position
- Turn ON and set averaging
- Turn ON and set smoothing

To run this program, you need:

- An established [GPIB interface connection](#)

### **See Other SCPI Example Programs**

```
GPIB.Write "SYSTem:PRESet"

'Select the measurement
GPIB.Write "CALCulate:PARAMeter:SElect 'CH1_S11_1'"

'Set the Data Format to Log Mag
GPIB.Write ":CALCulatel:FORMat MLOG"

'Turn ON the Trace, Title, and Frequency Annotation
GPIB.Write "DISplay:WINDow1:TRACel:STATe ON"
GPIB.Write "DISplay:WINDow1:TITLe:STATe ON"
GPIB.Write "DISplay:ANNotation:FREQuency ON"

'Autoscale the Trace
GPIB.Write "DISplay:WINDow1:TRACel:Y:Scale:AUTO"

'Query back the Per Division, Reference Level, and Reference Position
GPIB.Write "DISplay:WINDow1:TRACel:Y:SCALE:PDIVision?"
Pdiv = GPIB.Read
GPIB.Write "DISplay:WINDow1:TRACel:Y:SCALE:RLEVel?"
Rlev = GPIB.Read
GPIB.Write "DISplay:WINDow1:TRACel:Y:SCALE:RPOsition?"
Ppos = GPIB.Read

'Turn ON, and average five sweeps
GPIB.Write "SENSe1:AVERage:STATe ON"
GPIB.Write "SENSe1:AVERage:Count 5"

'Turn ON, and set 20% smoothing aperture
GPIB.Write "CALCulatel:SMOothing:STATe ON"
GPIB.Write "CALCulatel:SMOothing:APERture 20"
```



## Perform a Guided Calibration using SCPI

---

This example performs a Guided 2-Port or 4-port Calibration using ONE set of calibration standards or an ECAL module.

A measurement must first be set up with desired frequency range, power, and so forth, ready to be calibrated.

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file, such as Notepad, and save it on the PNA hard drive as \*.vbs.

[Learn how to setup and run the macro.](#)

---

### See Other SCPI Example Programs

---

```
Dim app
Dim scpi
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpIStringParser
' To perform 2-port cal, Uncomment TwoPortGuidedCal()
' Then comment FourPortGuidedCal()
'Do 2-port Cal
TwoPortGuidedCal()
'Do 4-port Cal
'FourPortGuidedCal

Sub TwoPortGuidedCal()
' Select the connectors
scpi.Execute("sens:corr:coll:guid:conn:port1 ""APC 3.5 female"" ")
scpi.Execute("sens:corr:coll:guid:conn:port2 ""APC 3.5 male"" ")
scpi.Execute("sens:corr:coll:guid:conn:port3 ""Not used"" ")
scpi.Execute("sens:corr:coll:guid:conn:port4 ""Not used"" ")
MsgBox("Connectors defined for Ports 1 and 2")
' Select the Cal Kit for each port being calibrated.
scpi.Execute("sens:corr:coll:guid:ckit:port1 ""85052D"" ")
scpi.Execute("sens:corr:coll:guid:ckit:port2 ""85052D"" ")
' To use an ECal module instead, comment out the above two lines
' and uncomment these two lines and use the part number printed
' on your module (which in our case was N4691-60004), followed
' by the word 'ECal'. Your ECal module must already be connected
' via USB to the PNA.
'scpi.Execute("sens:corr:coll:guid:ckit:port1 ""N4691-60004 ECal"" ")
'scpi.Execute("sens:corr:coll:guid:ckit:port2 ""N4691-60004 ECal"" ")
MsgBox("Cal kits defined for Ports 1 and 2")
' Initiate the calibration and query the number of steps
numSteps = GenerateSteps()
' Measure the standards, compute and apply the cal
MeasureAndComplete(numSteps)
End Sub

Sub FourPortGuidedCal()
' Select the connectors
scpi.Execute("sens:corr:coll:guid:conn:port1 ""APC 3.5 female"" ")
```

```

scpi.Execute("sens:corr:coll:guid:conn:port2 ""APC 3.5 female"" ")
scpi.Execute("sens:corr:coll:guid:conn:port3 ""APC 3.5 female"" ")
scpi.Execute("sens:corr:coll:guid:conn:port4 ""APC 3.5 female"" ")
MsgBox("Connectors defined for Ports 1 to 4")
' Select the Cal Kit for each port being calibrated.
scpi.Execute("sens:corr:coll:guid:ckit:port1 ""85052D"" ")
scpi.Execute("sens:corr:coll:guid:ckit:port2 ""85052D"" ")
scpi.Execute("sens:corr:coll:guid:ckit:port3 ""85052D"" ")
scpi.Execute("sens:corr:coll:guid:ckit:port4 ""85052D"" ")
' To use an ECal module instead, comment out the above four lines
' and uncomment these four lines and use the part number printed
' on your module (which in our case was N4431-60003), followed
' by the word 'ECal'. Your ECal module must already be connected
' via USB to the PNA.
'scpi.Execute("sens:corr:coll:guid:ckit:port1 ""N4431-60003 ECal"" ")
'scpi.Execute("sens:corr:coll:guid:ckit:port2 ""N4431-60003 ECal"" ")
'scpi.Execute("sens:corr:coll:guid:ckit:port3 ""N4431-60003 ECal"" ")
'scpi.Execute("sens:corr:coll:guid:ckit:port4 ""N4431-60003 ECal"" ")
MsgBox("Cal kits defined for Ports 1 to 4")
' Initiate the calibration and query the number of steps
numSteps = GenerateSteps()
' If your selected cal kit is not a 4-port ECal module which can
' mate to all 4 ports at once, then you may want to choose which
' thru connections to measure for the cal. You must measure at
' least 3 different thru paths for a 4-port cal (for greatest
' accuracy you can choose to measure a thru connection for all 6
' pairings of the 4 ports). If you omit this command, the default
' is to measure from port 1 to port 2, port 1 to port 3, and
' port 1 to port 4. For this example we select to measure
' from port 1 to port 2, port 2 to port 3, and port 2 to port 4.
scpi.Execute("sens:corr:coll:guid:thru:ports 1,2,2,3,2,4")
' Re-generate the connection steps to account for the thru changes
numSteps = GenerateSteps()
' Measure the standards, compute and apply the cal
MeasureAndComplete(numSteps)
End Sub

Function GenerateSteps()
' Initiate the calibration and query the number of steps
scpi.Execute("sens:corr:coll:guid:init")
GenerateSteps = scpi.Execute("sens:corr:coll:guid:steps?")
End Function

Sub MeasureAndComplete(numSteps)
MsgBox("Number of steps is " + CStr(numSteps))
' Measure the standards
For i = 1 To numSteps
step = "Step " + CStr(i) + " of " + CStr(numSteps)
strPrompt = scpi.Execute("sens:corr:coll:guid:desc? " + CStr(i))
MsgBox strPrompt, vbOKOnly, step
scpi.Execute("sens:corr:coll:guid:acq STAN" + CStr(i))
Next
' Conclude the calibration
scpi.Execute("sens:corr:coll:guid:save")
MsgBox ("Cal is done!")
End Sub

```





## Perform Guided ECal using SCPI

---

This VBScript program performs a Guided ECal Calibration. While this example is good to use as a starting point for Guided ECal, the [Guided comprehensive cal example](#) has some advanced features that are not in this program.

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Guided.vbs. [Learn how to setup and run the macro.](#)

```
' Performing a 2-port cal (Ports 1 and 2)
Dim app
Dim scpi

' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpiStringParser

' Specify the DUT connectors
' (for each connector of your DUT, one of the ECal module's ports must have
' that same connector, or else you cannot achieve the cal using that module).
scpi.Execute "sens:corr:coll:guid:conn:port1 ""APC 3.5 female"" "
scpi.Execute "sens:corr:coll:guid:conn:port2 ""APC 3.5 male"" "

' Note: If your PNA has more than 2 ports, you would need to uncomment
' one or both of these next two lines, to explicitly specify this is
' just a 2-port cal.
'scpi.Execute "sens:corr:coll:guid:conn:port3 ""Not used"" "
'scpi.Execute "sens:corr:coll:guid:conn:port4 ""Not used"" "
MsgBox "Connectors defined for Ports 1 and 2"

' Select the ECal module for each port being calibrated.
' Use the part number printed on your module (which in our case was N4691-60004),
' followed by the word 'ECal'. Your ECal module must already be connected
' via USB to the PNA.
scpi.Execute "sens:corr:coll:guid:ckit:port1 ""N4691-60004 ECal"" "
scpi.Execute "sens:corr:coll:guid:ckit:port2 ""N4691-60004 ECal"" "
MsgBox "Cal kits defined for Ports 1 and 2"

' Initiate the calibration and query the number of steps
scpi.Execute "sens:corr:coll:guid:init"
numSteps = scpi.Execute("sens:corr:coll:guid:steps?")
MsgBox "Number of steps is " + CStr(numSteps)

' Measure the standards
For i = 1 To numSteps
 step = "Step " + CStr(i) + " of " + CStr(numSteps)
 strPrompt = scpi.Execute("sens:corr:coll:guid:desc? " + CStr(i))
 MsgBox strPrompt, vbOKOnly, step
 scpi.Execute "sens:corr:coll:guid:acq STAN" + CStr(i)
Next

' Conclude the calibration
scpi.Execute "sens:corr:coll:guid:save"
MsgBox "Cal is done!"
```



## Perform Guided Mechanical Cal using SCPI

---

This VBScript program performs a Guided Calibration using Mechanical standards. While this example is good to use as a starting point for guided mechanical cal, the [Guided comprehensive cal example](#) has some advanced features that are not in this program.

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Guided.vbs. [Learn how to setup and run the macro.](#)

```
' Performing a 2-port cal (Ports 1 and 2)
```

```
Dim app
Dim scpi

' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpiStringParser

' Specify the DUT connectors
scpi.Execute "sens:corr:coll:guid:conn:port1 ""APC 3.5 female"" "
scpi.Execute "sens:corr:coll:guid:conn:port2 ""APC 3.5 male"" "

' Note: If your PNA has more than 2 ports, you would need to uncomment
' one or both of these next two lines, to explicitly specify this is
' just a 2-port cal.
'scpi.Execute "sens:corr:coll:guid:conn:port3 ""Not used"" "
'scpi.Execute "sens:corr:coll:guid:conn:port4 ""Not used"" "
MsgBox "Connectors defined for Ports 1 and 2"

' Select the Cal Kit for each port being calibrated.
scpi.Execute "sens:corr:coll:guid:ckit:port1 ""85052D"" "
scpi.Execute "sens:corr:coll:guid:ckit:port2 ""85052D"" "
MsgBox "Cal kits defined for Ports 1 and 2"

' Initiate the calibration and query the number of steps
scpi.Execute "sens:corr:coll:guid:init"
numSteps = scpi.Execute("sens:corr:coll:guid:steps?")
MsgBox "Number of steps is " + CStr(numSteps)

' Measure the standards
For i = 1 To numSteps
 step = "Step " + CStr(i) + " of " + CStr(numSteps)
 strPrompt = scpi.Execute("sens:corr:coll:guid:desc? " + CStr(i))
 MsgBox strPrompt, vbOKOnly, step
 scpi.Execute "sens:corr:coll:guid:acq STAN" + CStr(i)
Next

' Conclude the calibration
scpi.Execute "sens:corr:coll:guid:save"
MsgBox "Cal is done!"
```

## Perform a Guided 1-Port Cal on Port 2

---

This VBScript program does the following:

1. Clear measurements from the PNA
2. Create a new S22 measurement
3. Set an instrument state
4. Select the connector types
5. Select a cal kit
6. Initiate a Guided calibration
7. Display a prompt to connect each standard
8. Save the calibration to a newly created cal set

---

**Note:** This example illustrates an important step when calibrating a reflection measurement in the reverse direction. You **MUST** create a reverse (S22) measurement and have it be the active (selected) measurement on the channel that is being calibrated. This is not necessary for any calibrating any other measurement parameter.

---

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Guided.vbs. [Learn how to setup and run the macro.](#)

```
Dim App
Set App = CreateObject("AgilentPNA835x.Application")
App.Preset

Dim step
Dim Parser
Dim prompt
Dim txtDat
Dim Chan

Rem Clear old measurements
App.Reset

Rem Create a new Measurement
Set Parser = App.SCPIStringParser
Parser.Parse "DISPlay:WINDow1:STATE ON"
Parser.Parse "CALCulate:PARAMeter:DEFine 'MyMeas',S22"
Parser.Parse "DISPlay:WINDow1:TRACe1:FEED 'MyMeas'"

Rem Initialize state
Set Chan = App.ActiveChannel
Chan.StartFrequency = 200e6
Chan.StopFrequency = 1.5e9
Chan.IFBandwidth = 1000
step = 3
```

```

Rem Begin a guided calibration
Parser.Parse "SENS:CORR:COLL:GUID:CONN:PORT1 'Not used'"
Parser.Parse "SENS:CORR:COLL:GUID:CONN:PORT2 'Type N (50) male'"
Parser.Parse "SENS:CORR:COLL:GUID:CKIT:PORT1 '"
Parser.Parse "SENS:CORR:COLL:GUID:CKIT:PORT2 '85054D'"
Parser.Parse "SENS:CORR:COLL:GUID:INIT"

Rem Query the number of steps
txtDat = Parser.Parse("SENS:CORR:COLL:GUID:STEP?")

Rem Display the number of steps
MsgBox("Number of steps is " + txtDat)

Rem Set the loop counter limit
step = txtDat

Rem Measure the standards
For i = 1 To step
If i= 1 Then
prompt = Parser.Parse("sens:corr:coll:guid:desc? 1")
MsgBox(prompt)
Parser.Parse ("sens:corr:coll:guid:acq STAN1")
ElseIf i = 2 then
prompt = Parser.Parse("sens:corr:coll:guid:desc? 2")
MsgBox(prompt)
Parser.Parse ("sens:corr:coll:guid:acq STAN2")
ElseIf i = 3 then
prompt = Parser.Parse("sens:corr:coll:guid:desc? 3")
MsgBox(prompt)
Parser.Parse ("sens:corr:coll:guid:acq STAN3")
End If
Next

Rem All standards have been measured. Save the result
Parser.Parse "SENS:CORR:COLL:GUID:SAVE"
MsgBox("The calibration has been completed")

```

## Perform an Unguided ECal

---

This VBScript program performs an Unguided Full 2-Port ECal.

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Unguided.vbs. [Learn how to setup and run the macro.](#)

```
Set pna = CreateObject("AgilentPNA835x.Application")
Set scpi = pna.ScpIStringParser
' Preset the analyzer
scpi.Execute "SYSTem:PRESet"

' Start frequency of 10 MHz
scpi.Execute "SENSe:FREQUency:STARt 10E6"

' Stop frequency of 9 GHz
scpi.Execute "SENSe:FREQUency:STOP 9E9"

' Select the preset S11 measurement
scpi.Execute "CALCulate:PARAMeter:SElect 'CH1_S11_1'"
' Read the information about the Agilent factory
' characterization data of ECal module #1 on the USB bus
module1Info = scpi.Execute("SENSe:CORRection:COLlect:CKIT:INFormation? ECAL1,CHAR0")

' Prompt for the ECal module
MsgBox "Description of ECal Module #1:" & Chr(10) & Chr(10) & module1Info & _Chr(10)
& Chr(10) & "Make port connections to the ECal module, then press enter"
' ECal full 1 port and 2 port
' Choose a Calibration Type (comment out one of these)
scpi.Execute "SENSe:CORRection:COLlect:METhod refl3"
scpi.Execute "SENSe:CORRection:COLlect:METhod SPARSOLT"
' Specify to have the PNA automatically determine which port of the
' ECal module is connected to which port of the PNA.
scpi.Execute "SENSe:CORRection:PREFeRence:ECAL:ORientation ON"
' Alternatively, if you are measuring at very low power levels where
' the PNA fails to sense the module's orientation, you may need to turn
' off the auto orientation and specify how the module is connected (as in
' these next two commented lines of code -- "A1,B2" would indicate Port A
' of the module is connected to Port 1 and Port B is connected to Port 2).
'scpi.Execute "SENSe:CORRection:PREFeRence:ECAL:ORientation OFF"
'scpi.Execute "SENSe:CORRection:PREFeRence:ECAL:PMAP ECAL1,'A1,B2'"
' Acquire and store the calibration terms. *OPC? causes a "+1" to be
' returned when finished. CHAR0 indicates to use the Agilent factory
' characterized data within the ECal module (as opposed to a user characterization).
x = scpi.Execute("SENSe:CORRection:COLlect:ACQuire ECAL1,CHAR0;*OPC?")
MsgBox "Done with calibration."
```

## Perform an Unguided 2-Port Mechanical Cal

---

This VBScript program performs an Unguided, Full 2-Port, calibration using ONE set of mechanical calibration standards.

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Unguided.vbs. [Learn how to setup and run the macro.](#)

```
Set App = CreateObject("AgilentPNA835x.Application")
Set Scpi = App.SCPIStringParser

'Initialize state
Scpi.Execute ("SYSTEM:PRESet")

'Select the Preset measurement
Scpi.Execute ("CALCulate:PARAMeter:SElect 'CH1_S11_1'")

'Set the calibration method
Scpi.Execute ("SENSe:CORRection:COLLect:METHOD SPARSOLT")

'Select a cal kit
Scpi.Execute ("SENSe:CORRection:COLLect:CKIT:SElect 1")

'Set acquisition to FORWARD
Scpi.Execute ("SENSe:CORRection:SFORward ON")

'Measure the standards in forward direction
MsgBox "Connect OPEN to Port 1; then press OK"
Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan1")

MsgBox "Connect SHORT to Port 1; then press OK"
Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan2")

MsgBox "Connect LOAD to Port 1; then press OK"
Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan3")

'Set acquisition to REVERSE
Scpi.Execute ("SENSe:CORRection:SFORward OFF")

'Measure the standards in reverse direction
MsgBox "Connect OPEN to Port 2; then press OK"
Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan1")

MsgBox "Connect SHORT to Port 2; then press OK"
Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan2")

MsgBox "Connect LOAD to Port 2; then press OK"
Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan3")

'Measure the thru standard
MsgBox "Connect THRU between Ports 1 and 2; then press OK"
Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan4")
```



'OPTIONAL Measure Isolation

MsgBox "Connect LOADS to Port 1 AND Port 2; then press OK"

Scpi.Execute ("SENSe:CORRection:COLLect:ACQuire stan5")

'All standards have been measured. Save the result

Scpi.Execute ("SENS:CORR:COLL:SAVE")

MsgBox "The calibration has been completed"

## Perform an Unguided 1-Port Cal on Port 2

---

This VBScript program does the following:

1. Clear measurements from the PNA
2. Create a new S22 measurement
3. Set an instrument state
4. Select a cal kit
5. Initiate an Unguided calibration
6. Display a prompt to connect each standard
7. Save the calibration to a newly created cal set

---

**Note:** This example illustrates an important step when calibrating a reflection measurement in the reverse direction. You **MUST** create a reverse (S22) measurement and have it be the active (selected) measurement on the channel that is being calibrated. This is not necessary for any calibrating any other measurement parameter.

---

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Unguided.vbs. [Learn how to setup and run the macro.](#)

```
Dim App
Set App = CreateObject("AgilentPNA835x.Application")
App.Preset

Dim Parser
Dim Chan

Rem Clear old measurements
App.Reset

Rem Create a new Measurement
Set Parser = App.SCPIStringParser
Parser.Parse "DISPlay:WINDow1:STATE ON"
Parser.Parse "CALCulate:PARAMeter:DEFine 'MyMeas',S22"
Parser.Parse "DISPlay:WINDow1:TRACe1:FEED 'MyMeas'"

Rem Initialize state
Set Chan = App.ActiveChannel
Chan.StartFrequency = 200e6
Chan.StopFrequency = 1.5e9
Chan.IFBandwidth = 1000

Rem Begin an unguided calibration
Rem Set the calibration method
Parser.Parse "SENSE:CORREction:COLLect:METHOD REFL3"

Rem Turn off continuous sweep
Parser.Parse "INITiate:CONTinuous OFF"
```

```
Rem Select a cal kit
Parser.Parse "SENSe:CORRection:COLLect:CKIT:SElect 1"

Rem Measure the standards
MsgBox("Connect OPEN to port 2. Then press OK")
Parser.Parse ("sens:corr:coll:acq STAN1")

MsgBox("Connect SHORT to port 2. Then press OK")
Parser.Parse ("sens:corr:coll:acq STAN2")

MsgBox("Connect LOAD to port 2. Then press OK")
Parser.Parse ("sens:corr:coll:acq STAN3")

Rem All standards have been measured. Save the result
Parser.Parse "SENS:CORR:COLL:SAVE"

Rem Turn ON continuous sweep
Parser.Parse "INITiate:CONTInuous ON"
MsgBox("The calibration has been completed")
```

## ECALConfidence Check using SCPI

---

This Visual Basic program performs a complete ECAL confidence check.

To run this program, you need:

- An established GPIB interface connection
- Agilent's VISA or National Instrument's VISA installed on your PC
- The module visa32.bas added to your VB project.
- A form with two buttons: cmdRun and cmdQuit
- A calibrated S11 1-port or N-port measurement active on Channel 1
- Window 1 is visible

### See Other SCPI Example Programs

```
'Session to VISA Default Resource Manager
Private defRM As Long
'Session to PNA
Private vipNA As Long
'VISA function status return code
Private status As Long

Private Sub Form_Load()
 defRM = 0
End Sub

Private Sub cmdRun_Click()
'String to receive data from the PNA
Dim strReply As String * 200

' Open the VISA default resource manager
status = viOpenDefaultRM(defRM)
If (status < VI_SUCCESS) Then HandleVISAError

' Open a VISA session (vipNA) to the PNA at GPIB address 16.
status = viOpen(defRM, "GPIB0::16::INSTR", 0, 0, vipNA)
If (status < VI_SUCCESS) Then HandleVISAError

' Need to set the VISA timeout value to give all our GPIB Reads
' sufficient time to complete before a timeout error occurs.
' For this example, let's try setting the limit to
' 10000 milliseconds (10 seconds).
status = viSetAttribute(vipNA, VI_ATTR_TMO_VALUE, 10000)
If (status < VI_SUCCESS) Then HandleVISAError

' Get the catalog of all the measurements currently on Channel 1.
status = myGPIBwrite(vipNA, "CALC1:PAR:CAT?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBread(vipNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError

' If an S11 measurement named "MY_S11" doesn't already exist,
' then create it.
If InStr(strReply, "MY_S11") = 0 Then
 status = myGPIBwrite(vipNA, "CALC1:PAR:DEF MY_S11,S11")
```

```

 If (status < VI_SUCCESS) Then HandleVISAError
End If
strReply = ""

' Get the catalog of all the trace numbers currently active
' in Window 1.
status = myGPIBWrite(vipNA, "DISP:WIND1:CAT?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(vipNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError

' If a trace number 4 already exists in Window 1, then this
' will remove it.
If InStr(strReply, "4") > 0 Then
 status = myGPIBWrite(vipNA, "DISP:WIND1:TRAC4:DEL")
 If (status < VI_SUCCESS) Then HandleVISAError
End If

' Set trace number 4 to MY_S11.
status = myGPIBWrite(vipNA, "DISP:WIND1:TRAC4:FEED MY_S11")
If (status < VI_SUCCESS) Then HandleVISAError

' Set up trace view so we are viewing only the data trace.
status = myGPIBWrite(vipNA, "DISP:WIND1:TRAC4 ON")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBWrite(vipNA, "DISP:WIND1:TRAC4:MEM OFF")
If (status < VI_SUCCESS) Then HandleVISAError

' Select MY_S11 as the measurement to be used for the
' Confidence Check.
status = myGPIBWrite(vipNA, "SENS1:CORR:CCH:PAR MY_S11")
If (status < VI_SUCCESS) Then HandleVISAError

' Acquire the S11 confidence check data from ECal Module A
' into the memory buffer (asking for an OPC reply when it's done).
status = myGPIBWrite(vipNA, "SENS1:CORR:CCH:ACQ ECAL1;*OPC?")
If (status < VI_SUCCESS) Then HandleVISAError

' The PNA sends an OPC reply ("+1") when the confidence data
' acquisition into memory is complete, so this Read is waiting on
' the reply until it is received.
status = myGPIBRead(vipNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError

' Turn on trace math so the trace shows data divided by memory.
' You can be confident the S11 calibration is reasonably good if
' the displayed trace varies no more than a few tenths of a dB
' from 0 dB across the entire span.
status = myGPIBWrite(vipNA, "CALC1:MATH:FUNC DIV")
If (status < VI_SUCCESS) Then HandleVISAError
End Sub

Private Sub cmdQuit_Click()
' Turn off trace math
status = myGPIBWrite(vipNA, "CALC1:MATH:FUNC NORM")
If (status < VI_SUCCESS) Then HandleVISAError

```

```

' Conclude the confidence check to set the ECal module
' back to it's idle state.
status = myGPIBWrite(viPNA, "SENS1:CORR:CCH:DONE")
If (status < VI_SUCCESS) Then HandleVISAError

' Close the resource manager session (which also closes
' the session to the PNA).
If defRM <> 0 Then Call viClose(defRM)

' End the program
End
End Sub

Private Function myGPIBWrite(ByVal viHandle As Long, ByVal strOut As String) As Long
' The "+ Chr$(10)" appends an ASCII linefeed character to the output, for
' terminating the write transaction.
myGPIBWrite = viVPrintf(viHandle, strOut + Chr$(10), 0)
End Function

Private Function myGPIBRead(ByVal viHandle As Long, strIn As String) As Long
myGPIBRead = viVScanf(viHandle, "%t", strIn)
End Function

Sub HandleVISAError()
Dim strVisaErr As String * 200
Call viStatusDesc(defRM, status, strVisaErr)
MsgBox "*** Error : " + strVisaErr, vbExclamation
End
End Sub

```

## Perform a Source and Receiver Power Cal using SCPI

---

Programming the PNA using COM or using SICL/VISA over LAN (as in this example) leaves the PNA free to control GPIB devices as needed.

The first example, using Visual Basic, demonstrates the following:

- Performing a source power calibration of Port 2 for Channel 1.
- Reading the calibration data.

The second example performs a [Receiver Power Cal](#) using VBScript.

Learn more about [Power Calibrations](#).

See an example that [Uploads a Source Power Cal](#).

### Other SCPI Example Programs

To run this program, you need:

- One of the following power meters connected to the PNA through GPIB: E4416A, E4417A, E4418A/B, E4419A/B, 437B, 438A, EPM-441A, EPM-442A

---

**Note:** If your power meter is other than these, you can [create your own Power Meter Driver](#) using our template.

- Your PC and PNA both connected to a LAN (for communicating with each other).
- The SICL and VISA components of Agilent's I/O Libraries software installed on your PC (both are included when you install the software, unless you already have another vendor's VISA installed. Then specify Full SICL and VISA installation to overwrite the other vendor's VISA).
- The module visa32.bas added to your VB project.
- A form with two buttons: cmdRun and cmdQuit.
- A VISA interface configured on your remote PC to control the PNA. This could be GPIB interface or a [VISA LAN Client](#).

---

Note: The [SOURce:POWer:CORRection:COLLect:ACQuire](#) command, used to step the PNA and read a power meter, cannot be sent over the GPIB unless the power meter is connected to a different GPIB interface. See the alternative methods described in the command details.

---

```
'Session to VISA Default Resource Manager
Private defRM As Long
'Session to PNA
Private viPNA As Long
'VISA function status return code
Private status As Long

Private Sub Form_Load()
```

```

defRM = 0
End Sub

Private Sub cmdRun_Click()
' String to receive data from the PNA.
' Dimensioned large enough to receive scalar comma-delimited values
' for 21 frequency points (20 ASCII characters per point)
Dim strReply As String * 420

Dim strStimulus, strCalValue
Dim strResult As String

' Open the VISA default resource manager
status = viOpenDefaultRM(defRM)
If (status < VI_SUCCESS) Then HandleVISAError

' ' Open a session (vipNA) to the PNA at "address 16" on the VISA
' interface configured as "GPIB1" on this PC. This could be a
' VISA LAN Client pointing to the SIDL LAN Server on the PNA, or
' an actual GPIB interface on this PC connected to the PNA GPIB
' (in which case the power meter would need to be connected to a
' different GPIB interface on the PNA, such as the Agilent 82357A
' USB-to-GPIB).
status = viOpen(defRM, "GPIB0::16::INSTR", 0, 0, vipNA)
If (status < VI_SUCCESS) Then HandleVISAError

' Set the number of sweep points to 21 on Channel 1.
status = myGPIBWrite(vipNA, "SENS1:SWE:POIN 21")
If (status < VI_SUCCESS) Then HandleVISAError

' Specify the GPIB address of the power meter
' that will be used in performing the calibration.
status = myGPIBWrite(vipNA, "SYST:COMM:GPIB:PMET:ADDR 13")
If (status < VI_SUCCESS) Then HandleVISAError

' Turn use of the loss table OFF (this assumes there is
' virtually no loss in the RF path to the power sensor
' due to a splitter, coupler or adapter).
status = myGPIBWrite(vipNA, "SOUR:POW:CORR:COLL:TABL:LOSS OFF")
If (status < VI_SUCCESS) Then HandleVISAError

' Turn frequency checking OFF (so one power sensor is used for the entire cal
' acquisition sweep regardless of frequency span).
status = myGPIBWrite(vipNA, "SOUR:POW:CORR:COLL:FCH OFF")
If (status < VI_SUCCESS) Then HandleVISAError

' Specify a nominal power accuracy tolerance (NTolerance) in dB for the calibration,
' and the maximum number (COUNT) of iterations to adjust power at each point,
' attempting to achieve within tolerance of the desired power. If at any stimulus
' point the power fails to reach within the set tolerance of the desired power
' after the maximum number of iterations, the power at that point will be set to the
' value determined by the last iteration (the Source Power Cal dialog box will
' indicate the FAIL, but we can still apply the cal if desired when it's complete).
' Each iteration is based upon a SETTLED power reading (see comments preceding the
' next two commands below).
status = myGPIBWrite(vipNA, "SOUR1:POW2:CORR:COLL:ITER:NTOL 0.1")
If (status < VI_SUCCESS) Then HandleVISAError

```



```

status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:ITER:COUN 3")
If (status < VI_SUCCESS) Then HandleVISAError

' The worst-case window of power uncertainty (for a calibration which meets
' tolerance) is the sum of the iteration tolerance and the power meter settling
' tolerance (which is described below).

' At each stimulus point, the PNA takes power meter readings and determine when
' they have settled by comparing the magnitude difference between consecutive
' readings versus a nominal dB tolerance limit (NTOLerance) on that magnitude
' difference. When consecutive readings are within tolerance of each other, or
' if they are not within tolerance but we've taken a maximum number of readings
' (COUNT), the PNA does a weighted average of the readings taken at that stimulus
' point and that is considered our settled power reading.
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:AVER:NTOL 0.1")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:AVER:COUN 5")
If (status < VI_SUCCESS) Then HandleVISAError

' Specify if the cal power level is offset (positive value for a gain, negative
' value for a loss) from the PNA port power setting on the channel when no source
' power cal is active. This is to account for components between the PNA test
' port and cal reference plane. In this example, we will calibrate at the PNA
' test port, so there is no offset (it is zero).

status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:OFFS 0 DB")
If (status < VI_SUCCESS) Then HandleVISAError

' Specify the method (type of devices) that will be used to perform the cal.
' Choose either power meter (PMETer), or power meter and receiver (PMReceiver).
' PMReceiver uses the power meter for the first iteration of each point and
' the PNA's reference receiver for subsequent iterations, so is much faster
' than using power meter only. But the power meter accounts for compression
' when calibrating at the output of an active device, whereas the reference
' receiver cannot unless it is coupled to the cal reference plane (on a PNA
' which allows direct access to the receivers).
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:METH PMET")
'status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:METH PMR")
If (status < VI_SUCCESS) Then HandleVISAError

' Show the source power cal dialog during the source power cal acquisition.
' (this is the default, so this command is only necessary if this setting
' may have been changed beforehand, perhaps by another program).
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:DISP ON")
If (status < VI_SUCCESS) Then HandleVISAError

' Perform the source power cal acquisition sweep using the sensor attached to
' Channel A of the power meter (asking for an OPC reply when it's done). This
' assumes that the power sensor is already connected to Port 2 of the PNA.
' We'll put up an hourglass cursor while waiting for the acquire to complete.
Screen.MousePointer = vbHourglass
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:ACQ ASEN;*OPC?")
If (status < VI_SUCCESS) Then HandleVISAError

' In the process of beginning a source power cal acquisition, the PNA searches
' for the power meter on VISA interfaces configured in the Agilent I/O Libraries
' on the PNA. One of those interfaces is the SICL/VISA LAN server, so if this

```

```

' program is using that interface, we need to ensure our program is not pending
' an operation on that interface when the PNA wants to search it. So this
' Wait subroutine suspends execution of our program (for 6000 milliseconds =
' 6 seconds), giving the PNA time to search that interface and discover that the
' power meter is not there (the 6 seconds is just to be safe, the search actually
' takes only a few seconds).
' Note: If instead of using the VISA LAN server interface, you are having this
' program communicate with the PNA via it's GPIB interface (which requires the
' power meter be connected to a different GPIB interface on the PNA, such as the
' Agilent 82357A USB-to-GPIB), then this Wait is not needed.
Wait 6000

' The PNA sends an OPC reply ("+1") when the cal acquisition is complete, so
' our Read operation will wait on the reply until it is received. We need to
' set the VISA timeout value long enough to give our Read sufficient time to
' complete before a timeout error occurs. For this example, let's try setting
' the limit to 60000 milliseconds (60 seconds).
status = viSetAttribute(viPNA, VI_ATTR_TMO_VALUE, 60000)
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(viPNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError

' Change mouse cursor from hourglass back to normal
Screen.MousePointer = vbDefault

' Conclude the calibration. This applies the cal data to PNA channel memory,
' and turns the correction ON for Port 2 on Channel 1,
' but does NOT save the calibration.
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:COLL:SAVE")
If (status < VI_SUCCESS) Then HandleVISAError

' At this point, if you choose to save the instrument state as a ".CST" file,
' the calibration will be saved with the instrument state in that file.

' Prepare for doing data transfer in ASCII format.
status = myGPIBWrite(viPNA, "FORM:DATA ASCII")
If (status < VI_SUCCESS) Then HandleVISAError

' Read the stimulus values from Channel 1.
status = myGPIBWrite(viPNA, "SENS1:X?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(viPNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError

' Tokenize the reply string into an array containing the values
strStimulus = Split(strReply, ",")

' Read the source power correction data.
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:DATA?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(viPNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError

' Tokenize the reply string into an array containing the values
strCalValue = Split(strReply, ",")

' Print the data using a message box (here, Chr returns the ASCII characters

```

```

' for Tab (9) and Linefeed (10)).
strResult = "Stimulus" & Chr(9) & Chr(9) & "Cal Value" & Chr(10)
For i = 0 To UBound(strStimulus)
strResult = strResult & Val(strStimulus(i)) & Chr(9) & Val(strCalValue(i)) & Chr(10)
Next
MsgBox strResult
End Sub

Private Function myGPIBWrite(ByVal viHandle As Long, ByVal strOut As String) As Long

' The "+ Chr$(10)" appends an ASCII linefeed character to the
' output, for terminating the write transaction.
myGPIBWrite = viVPrintf(viHandle, strOut + Chr$(10), 0)
End Function

Private Function myGPIBRead(ByVal viHandle As Long, strIn As String) As Long
myGPIBRead = viVScanf(viHandle, "%t", strIn)
End Function

Sub HandleVISAError()
Dim strVisaErr As String * 200
Call viStatusDesc(defRM, status, strVisaErr)
MsgBox "****Error : " + strVisaErr, vbExclamation

' Close the resource manager session (which also closes
' the session to the PNA).

If defRM <> 0 Then Call viClose(defRM)
End
End Sub

Public Sub Wait(ByVal mS_delay As Long)

Dim t0 As Single
t0 = Timer
Do While Timer - t0 < mS_delay / 1000
Dim dummy As Integer
dummy = DoEvents() ' if we cross midnight, back up one day
If Timer < t0 Then t0 = t0 - 86400
Loop
End Sub

```

### Perform a Receiver Power Cal

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file, such as Notepad, and save it on the PNA hard drive as \*.vbs.

[Learn how to setup and run the macro.](#)

```

Dim pna
Dim scpi
Set pna = CreateObject("AgilentPNA835x.Application")
Set scpi = pna.ScpiStringParser

```

```

' For simplicity, this example starts from the preset instrument state
scpi.Execute "SYST:PRESet"
' Turn off continuous sweep
scpi.Execute "INITiate:CONTinuous OFF"
' Select the S11 measurement that was created by the instrument preset
scpi.Execute "CALCulate:PARAMeter:SElect 'CH1_S11_1'"
' Change the measurement parameter to measure the B receiver
scpi.Execute "CALCulate:PARAMeter:MODify B,1"
' Specify the Calibration Type, then Prompt
' to ensure the receiver is connected to port 1.
scpi.Execute "SENSE:CORRection:COLLect:METHOD RPOwer"
MsgBox "Connect port 1 to port 2 so power is supplied to the B receiver, then press
enter"
' Acquire the power measurement; returning reply to *OPC? when finished.
response = scpi.Execute("SENSE:CORRection:COLLect:ACQuire POWer;*OPC?")
' Compute the error term, store to calset and turn on the calibration.
response = scpi.Execute("SENSE:CORRection:COLLect:SAVE")
MsgBox "Done with calibration."

```

## Uploading a Source Power Cal using SCPI

---

Programming the PNA using COM or using SICL/VISA over LAN (as in this example) leaves the PNA free to control GPIB devices as needed. This Visual Basic program demonstrates:

- Uploading a source power calibration of Port 2 for Channel 1.
- Reading the calibration data.

Learn more about [Power Calibrations](#)

### Other SCPI Example Programs

To run this program, you need:

- Your PC and PNA both connected to a LAN (if using VISA LAN server / client).
- The SICL and VISA components of Agilent's I/O Libraries software installed on your PC (both are included when you install the software, unless you already have another vendor's VISA installed. Then specify Full SICL and VISA installation to overwrite the other vendor's VISA).
- The module visa32.bas added to your VB project.
- A form with two buttons: cmdRun and cmdQuit.
- A VISA interface configured on your remote PC to control the PNA. This could be GPIB interface or a [VISA LAN Client](#).

```
'Session to VISA Default Resource Manager
Private defRM As Long
'Session to PNA
Private viPNA As Long
'VISA function status return code
Private status As Long
Private Sub Form_Load()
defRM = 0
End Sub
Private Sub cmdRun_Click()

' String to receive data from the PNA.
' Dimensioned large enough to receive scalar comma-delimited values
' for 21 frequency points (20 ASCII characters per point)
Dim strReply As String * 420
Dim strPower As String, strCalPower As String
Dim strStimulus, strCalValue
Dim strResult As String

' Open the VISA default resource manager
status = viOpenDefaultRM(defRM)
If (status < VI_SUCCESS) Then HandleVISAError

' Open a session (viPNA) to the PNA at "address 16" on the VISA
' interface configured as "GPIB0" on this PC.
```

```

status = viOpen(defRM, "GPIB0::16::INSTR", 0, 0, vipNA)
If (status < VI_SUCCESS) Then HandleVISAError

' Set the number of sweep points to 2 on Channel 1.
status = myGPIBWrite(vipNA, "SENS1:SWE:POIN 2")
If (status < VI_SUCCESS) Then HandleVISAError

' Ensure there's currently no source power cal on for this channel and port.
status = myGPIBWrite(vipNA, "SOUR1:POW2:CORR OFF")
If (status < VI_SUCCESS) Then HandleVISAError

' Specify if the cal power level is offset (positive value for a gain, negative
' value for a loss) from the PNA port power setting on the channel when no source
' power cal is active. This is to account for components between the PNA test
' port and cal reference plane. In this example, let's set up our calibration
' at the output of an amplifier with 15 dB gain.
status = myGPIBWrite(vipNA, "SOUR1:POW2:CORR:OFFS 15 DB")
If (status < VI_SUCCESS) Then HandleVISAError

' Prepare for doing data transfer in ASCII format.
status = myGPIBWrite(vipNA, "FORM:DATA ASCII")
If (status < VI_SUCCESS) Then HandleVISAError

' Send our source power correction data to the PNA. For purpose of simplicity
' in this example, we'll set up for no correction (0) at our start stimulus and
' 0.5 dB at our stop stimulus (recall that our sweep currently has just 2 points).
status = myGPIBWrite(vipNA, "SOUR1:POW2:CORR:DATA 0,0.5")
If (status < VI_SUCCESS) Then HandleVISAError

' Set the number of sweep points to 21 on Channel 1.
status = myGPIBWrite(vipNA, "SENS1:SWE:POIN 21")
If (status < VI_SUCCESS) Then HandleVISAError

' Read the fixed power level for this port on Channel 1.
status = myGPIBWrite(vipNA, "SOUR1:POW2:LEV?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(vipNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError
strPower = strReply

' Turn the source power cal on.
status = myGPIBWrite(vipNA, "SOUR1:POW2:CORR ON")
If (status < VI_SUCCESS) Then HandleVISAError

' Again read the fixed power level for this port on Channel 1
' (with our calibration turned on, this should now include the 15 dB offset
' we indicated our power amplifier provides).
status = myGPIBWrite(vipNA, "SOUR1:POW2:LEV?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(vipNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError
strCalPower = strReply

' Read the stimulus values from Channel 1.
status = myGPIBWrite(vipNA, "SENS1:X?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(vipNA, strReply)

```

```

If (status < VI_SUCCESS) Then HandleVISAError

' Tokenize the reply string into an array containing the values
strStimulus = Split(strReply, ",")

' Read back the source power correction data, now interpolated for 21 points
status = myGPIBWrite(viPNA, "SOUR1:POW2:CORR:DATA?")
If (status < VI_SUCCESS) Then HandleVISAError
status = myGPIBRead(viPNA, strReply)
If (status < VI_SUCCESS) Then HandleVISAError

' Tokenize the reply string into an array containing the values
strCalValue = Split(strReply, ",")

' Print the data using a message box (here, Chr returns the ASCII characters
' for Tab (9) and Linefeed (10)).
strResult = "PNA port power = " & Val(strPower) & Chr(10)
strResult = strResult & "Power at reference plane = " & Val(strCalPower) & Chr(10)
Chr(10)
strResult = strResult & "Stimulus" & Chr(9) & Chr(9) & "Cal Value" & Chr(10)
For i = 0 To UBound(strStimulus)
 strResult = strResult & Val(strStimulus(i)) & Chr(9) & Val(strCalValue(i)) &
Chr(10)
Next
MsgBox strResult
End Sub
Private Sub cmdQuit_Click()

' Close the resource manager session (which also closes
' the session to the PNA).
If defRM <> 0 Then Call viClose(defRM)

' End the program
End
End Sub
Private Function myGPIBWrite(ByVal viHandle As Long, ByVal strOut As String) As Long

' The "+ Chr$(10)" appends an ASCII linefeed character to the
' output, for terminating the write transaction.
myGPIBWrite = viVPrintf(viHandle, strOut + Chr$(10), 0)
End Function
Private Function myGPIBRead(ByVal viHandle As Long, strIn As String) As Long
myGPIBRead = viVScanf(viHandle, "%t", strIn)

' Remove trailing linefeed character
If Right(strIn, 1) = Chr(10) Then strIn = Left(strIn, Len(strIn) - 1)
End Function
Sub HandleVISAError()
Dim strVisaErr As String * 200
Call viStatusDesc(defRM, status, strVisaErr)
MsgBox "*** Error : " + strVisaErr, vbExclamation

' Close the resource manager session (which also closes
' the session to the PNA).
If defRM <> 0 Then Call viClose(defRM)
End
End Sub

```





## Perform a Sliding Load Calibration using GPIB

---

This Visual Basic program does a **only** the sliding load portion of a Calibration.  
To run this program, you need:

- An established GPIB interface connection
- A measurement and calibration routine to call this sub-program
- STAN3 set up as a sliding load standard

### See Other SCPI Example Programs

```
Sub slide()
'Measure the sliding load for at least 5 and no more than 7 slides
'Note that "SLSET" and "SLDONE" must be executed before the actual acquisition of a
slide
MsgBox "Connect Sliding Load; set to Position 1; then press OK"
GPIB.Write "SENS:CORR:COLL SLSET"
GPIB.Write "SENS:CORR:COLL STAN3;"

MsgBox "Set Sliding Load to position 2; then press OK"
GPIB.Write "SENS:CORR:COLL SLSET"
GPIB.Write "SENS:CORR:COLL STAN3;"

MsgBox "Set Sliding Load to position 3; then press OK"
GPIB.Write "SENS:CORR:COLL SLDONE"
GPIB.Write "SENS:CORR:COLL STAN3;"
End Sub
```

## Create New Cal Kit using SCPI

---

When creating new cal kits programmatically, the order in which cal kit commands are sent can be important. For example to create a kit with opens, shorts, loads, and thrus. Be sure to use the following sequence for each newly defined standard.

1. Programmatically select the standard number
2. Programmatically select the standard type.
3. Program the cal standard's values.
4. Repeat steps 1, 2, 3 for additional new standards being defined.

```
10 !
20 !
30 ! This example program demonstrates how to create
40 ! new PNA calibration kits.
50 !
60 ! 1) Select a kit not previously defined
70 ! 2) Define open, short, load, and thru cal standards
80 ! Note: Each of the newly defined standards is assigned
90 ! a default connector name. These default connector names
100 ! will be replaced in subsequent steps.
110 ! 3) Use the delete connector command to remove default
120 ! connector names.
130 ! 4) Add connectors. Specify:
140 ! Start and Stop Freq
150 ! Z - Impedance
160 ! sex - MALE, FEMALE, NONE
170 ! media - COAX, WAVE
180 ! cutoff - Frequency for waveguide
190 ! 5) Assign the appropriate connector to each standard
200 ! 6) Modify the class assignments for the standards defined
210 ! 7) Verify the kit values
220 !
230 ! Additional Note: After setting each new cal kit value, it is
240 ! recommended that the program periodically perform queries to
250 ! verify the new values.
260 !
270 ! This will prevent program synchronization issues that can affect
280 ! final values stored within new cal kits.
290 !
300 !-----
310 !
320 ! Set up I/O path
330 ASSIGN @Na TO 716
340 DIM Calkname${80},Conn${80}
350 INTEGER Calkitnum
360 !
370 CLEAR SCREEN
380 !
390 !!!
```

```

400 ! Designate the kit selection to be used for performing cal's
410 OUTPUT @Na;":sens:corr:ckit:count?"
420 ENTER @Na;Calkitnum
430 Calkitnum=Calkitnum+1
440 OUTPUT @Na;":sens:corr:coll:ckit "&VAL$(Calkitnum)
450 !
460 ! Name this kit with your own name
470 OUTPUT @Na;":sens:corr:coll:ckit:name "Special 2.4 mm Model 85056""
480 !
490 !
500 DISP "Defining kit std 1..."
510 ! Now set up standard #1
520 OUTPUT @Na;":sens:corr:coll:ckit:stan 1"
530 OUTPUT @Na;":sens:corr:coll:ckit:stan:type SHORT"
540 Get_std
550 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
560 OUTPUT @Na;":sens:corr:coll:ckit:stan:label "My Short""
570 Get_label
580 !
590 DISP "Defining kit std 2..."
600 ! Now set up standard #2
610 OUTPUT @Na;":sens:corr:coll:ckit:stan 2"
620 OUTPUT @Na;":sens:corr:coll:ckit:stan:type OPEN"
630 Get_std
640 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
650 OUTPUT @Na;":sens:corr:coll:ckit:stan:label "My Open""
660 Get_label
670 !
680 DISP "Defining kit std 3..."
690 ! Now set up standard #3
700 OUTPUT @Na;":sens:corr:coll:ckit:stan 3"
710 OUTPUT @Na;":sens:corr:coll:ckit:stan:type LOAD"
720 Get_std
730 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
740 OUTPUT @Na;":sens:corr:coll:ckit:stan:label "My Fixed Load""
750 Get_label
760 !
770 DISP "Defining kit std 4..."
780 ! Now set up standard #4
790 OUTPUT @Na;":sens:corr:coll:ckit:stan 4"
800 OUTPUT @Na;":sens:corr:coll:ckit:stan:type THRU"
810 Get_std
820 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
830 OUTPUT @Na;":sens:corr:coll:ckit:stan:label "My Thru""
840 Get_label
850 !
860 DISP "Defining kit std 5..."
870 ! Now set up standard #5
880 OUTPUT @Na;":sens:corr:coll:ckit:stan 5"
890 OUTPUT @Na;":sens:corr:coll:ckit:stan:type SLOAD"
900 Get_std
910 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
920 OUTPUT @Na;":sens:corr:coll:ckit:stan:label "Sliding Load""

```

```

930 Get_label
940 !
950 DISP "Defining kit std 6..."
960 ! Now set up standard #6
970 !
980 OUTPUT @Na;":sens:corr:coll:ckit:stan 6"
990 OUTPUT @Na;":sens:corr:coll:ckit:stan:type SHORT"
1000 Get_std
1010 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
1020 OUTPUT @Na;":sens:corr:coll:ckit:stan:label ""Short""
1030 Get_label
1040 !
1050 DISP "Defining kit std 7..."
1060 ! Now set up standard #7
1070 OUTPUT @Na;":sens:corr:coll:ckit:stan 7"
1080 OUTPUT @Na;":sens:corr:coll:ckit:stan:type SHORT"
1090 Get_std
1100 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
1110 OUTPUT @Na;":sens:corr:coll:ckit:stan:label ""Short""
1120 Get_label
1130 !
1140 DISP "Defining kit std 8..."
1150 ! Now set up standard #8
1160 !
1170 OUTPUT @Na;":sens:corr:coll:ckit:stan 8"
1190 OUTPUT @Na;":sens:corr:coll:ckit:stan:type ARBI"
1200 Get_std
1210 OUTPUT @Na;":sens:corr:coll:ckit:stan:char coax"
1220 OUTPUT @Na;":sens:corr:coll:ckit:stan:TZR 15;"
1230 OUTPUT @Na;":sens:corr:coll:ckit:stan:TZI -9;"
1240 OUTPUT @Na;":sens:corr:coll:ckit:stan:label ""Z Load""
1250 Get_label
1260 !
1270 !
1280 !
1290 ! First remove any old connector names
1300 OUTPUT @Na;":sens:corr:coll:ckit:conn:del"
1310 ! Verify that no connectors are currently installed
1320 OUTPUT @Na;":sens:corr:coll:ckit:conn:cat?"
1330 ENTER @Na;Conn$
1340 PRINT "Verify empty list: ";Conn$
1350 !
1360 ! Define your new connectors
1370 OUTPUT @Na;":sens:corr:coll:ckit:conn:add ""PSC
2.4""",0HZ,999GHZ,50.0,MALE,COAX,0.0"
1380 OUTPUT @Na;":sens:corr:coll:ckit:conn:add ""PSC
2.4""",0HZ,999GHZ,50.0,FEMALE,COAX,0.0"
1390 !
1400 ! Verify that the new connectors are installed
1410 OUTPUT @Na;":sens:corr:coll:ckit:conn:cat?"
1420 ENTER @Na;Conn$
1430 PRINT "Verify new connectors: ";Conn$
1440 DISP ""

```

```

1450 !
1460 DISP "Defining conn std 1..."
1470 ! Now set up standard #1
1480 OUTPUT @Na;":sens:corr:coll:ckit:stan 1"
1490 Verify_std
1500 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",FEMALE,1"
1510 Print_connector
1520 !
1530 DISP "Defining conn std 2..."
1540 ! Now set up standard #2
1550 OUTPUT @Na;":sens:corr:coll:ckit:stan 2"
1560 Verify_std
1570 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",FEMALE,1"
1580 Print_connector
1590 !
1600 DISP "Defining conn std 3..."
1610 ! Now set up standard #3
1620 OUTPUT @Na;":sens:corr:coll:ckit:stan 3"
1630 Verify_std
1640 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",FEMALE,1"
1650 Print_connector
1660 !
1670 DISP "Defining conn std 4..."
1680 ! Now set up standard #4
1690 OUTPUT @Na;":sens:corr:coll:ckit:stan 4"
1700 Verify_std
1710 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",FEMALE,1"
1720 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",MALE,2"
1730 Print_connector
1740 !
1750 DISP "Defining conn std 5..."
1760 ! Now set up standard #5
1770 OUTPUT @Na;":sens:corr:coll:ckit:stan 5"
1780 OUTPUT @Na;":sens:corr:coll:ckit:stan:label "Sliding Load""
1790 Verify_std
1800 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",MALE,1"
1810 Print_connector
1820 !
1830 DISP "Defining conn std 6..."
1840 ! Now set up standard #6
1850 !
1860 OUTPUT @Na;":sens:corr:coll:ckit:stan 6"
1870 Verify_std
1880 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",MALE,1"
1890 Print_connector
1900 !
1910 DISP "Defining conn std 7..."
1920 ! Now set up standard #7
1930 OUTPUT @Na;":sens:corr:coll:ckit:stan 7"
1940 Verify_std
1950 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4",MALE,1"
1960 Print_connector
1970 !

```

```

1980 DISP "Defining conn std 8..."
1990 ! Now set up standard #8
2000 OUTPUT @Na;":sens:corr:coll:ckit:stan 8"
2010 Verify_std
2020 OUTPUT @Na;":sens:corr:coll:ckit:conn:snam "PSC 2.4","MALE,1"
2030 Print_connector
2040 !
2050 DISP "Class assignments..."
2060 !
2070 ! Designate the "order" associated with measuring the standards
2080 !
2090 ! Set Port 1, 1st standard measured to be standard #2
2100 OUTPUT @Na;":sens:corr:coll:ckit:order1 2"
2110 ! Set Port 1, 2nd standard measured to be standard #1
2120 OUTPUT @Na;":sens:corr:coll:ckit:order2 1,6,7"
2130 ! Set Port 1, 3rd standard measured to be standard #3 and #5
2140 OUTPUT @Na;":sens:corr:coll:ckit:order3 3,5"
2150 ! Set Port 1, 4th standard measured to be standard #4
2160 OUTPUT @Na;":sens:corr:coll:ckit:order4 4"
2170 !
2180 ! Set Port 2, 1st standard measured to be standard #2
2190 OUTPUT @Na;":sens:corr:coll:ckit:order5 2"
2200 ! Set Port 2, 2nd standard measured to be standard #1
2210 OUTPUT @Na;":sens:corr:coll:ckit:order6 1,6,7"
2220 ! Set Port 2, 3rd standard measured to be standard #3 and #6
2230 OUTPUT @Na;":sens:corr:coll:ckit:order7 3,5"
2240 ! Set Port 2, 4th standard measured to be standard #4
2250 OUTPUT @Na;":sens:corr:coll:ckit:order8 4"
2260 !
2270 ! Set Port 1, 1st standard
2280 OUTPUT @Na;":sens:corr:coll:ckit:olabel1 "MyOpen1""
2290 ! Set Port 1, 2nd standard
2300 OUTPUT @Na;":sens:corr:coll:ckit:olabel2 "MyShorts1""
2310 ! Set Port 1, 3rd standard
2320 OUTPUT @Na;":sens:corr:coll:ckit:olabel3 "MyLoads1""
2330 ! Set Port 1, 4th standard measured to be standard #4
2340 OUTPUT @Na;":sens:corr:coll:ckit:olabel4 "MyThru1""
2350 !
2360 ! Set Port 2, 1st standard
2370 OUTPUT @Na;":sens:corr:coll:ckit:olabel5 "MyOpen2""
2380 ! Set Port 2, 2nd standard
2390 OUTPUT @Na;":sens:corr:coll:ckit:olabel6 "MyShorts2""
2400 ! Set Port 2, 3rd standard
2410 OUTPUT @Na;":sens:corr:coll:ckit:olabel7 "MyLoads2""
2420 ! Set Port 2, 4th standard
2430 OUTPUT @Na;":sens:corr:coll:ckit:olabel8 "MyThrus2""
2440 !
2450 BEEP
2460 DISP "Done!"
2470 END
2480 SUB Get_label
2490 OUTPUT 716;":sens:corr:coll:ckit:stan:label?"
2500 ENTER 716;Label$

```

```
2510 PRINT Label$
2520 SUBEND
2530 !
2540 SUB Get_std
2550 OUTPUT 716;":sens:corr:coll:ckit:stan:type?"
2560 ENTER 716;Type$
2570 PRINT Type$
2580 SUBEND
2590 !
2600 SUB Print_connector
2610 DIM Nam$[40]
2620 OUTPUT 716;":sens:corr:coll:ckit:conn:sname?"
2630 ENTER 716;Nam$
2640 PRINT Nam$
2650 SUBEND
2660 !
2670 SUB Verify_std
2680 OUTPUT 716;":sens:corr:coll:ckit:stan:label?"
2690 ENTER 716;Label$
2700 SUBEND
2710 !
```

## Modify a Calibration Kit using SCPI

---

This Visual Basic program:

- Modifies Calibration kit number 3
- Completely defines standard #4 (thru)

To run this program, you need:

- An established GPIB interface connection

### See Other SCPI Example Programs

---

```
'Modifying cal kit number 3
Calkitnum = 3

'Designate the kit selection to be used for performing cal's
GPIB.Write "SENSE:CORREction:COLLect:CKIT:SElect " & Val(Calkitnum)

'Reset to factory default values.
GPIB.Write "SENSE:CORREction:COLLect:CKIT:RESet " & Val(Calkitnum)

'Name this kit with your own name
GPIB.Write "SENSe:CORREction:COLLect:CKIT:NAME 'My Cal Kit'"

'Assign standard numbers to calibration classes
'Set Port 1, class 1 (S11A) to be standard #8
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer1 8"
'Set Port 1, class 2 (S11B) to be standard #7
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer2 7"
'Set Port 1, class 3 (S11C) to be standard #3
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer3 3"
'Set Port 1, class 4 (S21T) to be standard #4
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer4 4"
'Set Port 2, class 1 (S22A) to be standard #8
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer5 8"
'↑ Set Port 2, class 2 (S22B) to be standard #7
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer6 7"
'Set Port 2, class 3 (S22C) to be standard #3
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer7 3"
'Set Port 2, class 4 (S12T) to be standard #4
GPIB.Write "SENSE:CORREction:COLLect:CKIT:ORDer8 4"

'Set up Standard #4 completely
'Select Standard #4; the rest of the commands act on it
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard 4"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:FMIN 300KHz"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:FMAX 9GHz"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:IMPedance 50"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:DELAy 1.234 ns"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:LOSS 23e6"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:C0 0"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:C1 1"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:C2 2"
GPIB.Write "SENSE:CORREction:COLLect:CKIT:STANdard:C3 3"
```



```
GPIB.Write "SENSe:CORRection:COLLect:CKIT:STANdard:L0 10"
GPIB.Write "SENSe:CORRection:COLLect:CKIT:STANdard:L1 11"
GPIB.Write "SENSe:CORRection:COLLect:CKIT:STANdard:L2 12"
GPIB.Write "SENSe:CORRection:COLLect:CKIT:STANdard:L3 13"
GPIB.Write "SENSe:CORRection:COLLect:CKIT:STANdard:LABel 'My Special Thru'"
GPIB.Write "SENSe:CORRection:COLLect:CKIT:STANdard:TYPE THRU"
GPIB.Write "SENSe:CORRection:COLLect:CKIT:STANdard:CHARacteristic Coax"
```

## Create and Calibrate a VMC Measurement

---

This VB Script example creates and calibrates a Vector mixer measurement. To run this example **without modification** you need the following:

- A Mixer setup file saved on the PNA: C:\Program Files\Agilent\Network Analyzer\Documents\Mixer\MyMixer.mxr.
- If the mixer file uses an external LO source, it must also be attached and configured.
- An ECAL module that covers the frequency range of the measurement.

The SCPI commands in this example are sent over a COM interface using the SCPIStringParser object. You do NOT need a GPIB connection to run this example. However, some modification may be necessary to make the program run on a traditional GPIB Interface.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as VMC.vbs. Learn how to setup and run the macro.

```
Dim app
Dim scpi
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpiStringParser
'---Create a Vector Mixer Measurement
'First, delete all measurements on the channel
scpi.Execute "CALC:PAR:DEL:ALL"
'Create a forward scalar mixer measurement and configure
'it in channel 1.
'The first parameter is a unique identifying string
'(specified by the user) to allow subsequent
'commands to be directed at this specific measurement.
SCPI.Execute "CALC:CUST:DEF "My VC21", "FCA.VMCMeas""
'Setup the new measurement as the 2nd trace in the active window
SCPI.Execute "DISP:WIND:TRAC2:FEED "My VC21""
'Make the new trace the active measurement
SCPI.Execute "CALC:PAR:SEL "My VC21""
'The parameters of the mixer measurement can now be configured.
'This can be done by either using the SENS:MIX commands
'for each of the parameters or by loading a mixer setup file.
'This example loads a mixer setup file. The path name
'for the mixer file may be loaded from other mapped drives.
SCPI.Execute "SENS:MIXer:Load "C:\Program Files\Agilent\Network
Analyzer\Documents\Mixer\MyMixer.mxr""

'-----Perform A Vector Mixer Calibration-----
'Initialize an VMC guided calibration for session number 6
SCPI.Execute "SENS:CORR:COLL:SESS6:INIT "VMC""
'This sets the VMC operation to full system cal as opposed to
'performing a mixer characterization only.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:OPER "CAL""
'This example uses ECAL for the 2-port cal portion of the procedure
'To use a mechanical kit you will have to use the following command:
'SCPI.Execute "SENS:CORR:COLL:SESS6:SMC:TWOport:OPTion "MECH""
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOport:OPTion "ECAL""
'If you select the mechanical method then you also have to
```

```

'specify the connector types and the cal kits for each of the ports.
'The comments below show an example of how that is done:
'SCPI.Execute "SENS:CORR:COLL:SESS6:CONN:PORT1:SEL ""APC 3.5 male""
'SCPI.Execute "SENS:CORR:COLL:SESS6:CONN:PORT2:SEL ""APC 3.5 female""
'SCPI.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT1:SEL ""85052D""
'SCPI.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT2:SEL ""85052D""
'Choose the between ECal or Mechanical calibration for the
'Mixer Characterization portion of the VMC cal.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:MIX:CHAR:CAL:OPT ""ECAL""
'This command sets the port mapping for the ECal to be used
'during the Mixer Characterization portion of the VMC cal.
'It is a required command if in the previous command the option
'was set to 'ECAL'. The only valid port maps are either 'A1'
'or 'B1'.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:MIX:ECAL:PORT 1, ""A1""
'Specify the ECal module and the ECal characterization for the
'two port calibration portion of this session. FCA calibrations
'currently only support ECal module number 1. In this example
'the factory characterization is used by specifying 0 for the
'characterization number.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:ECAL:CHAR 1,0"
'Specify the ECal module and the ECal characterization for the
'Mixer Characterization portion of this session. FCA calibrations
'currently only support ECal module number 1. In this example
'the factory characterization is used by specifying 0 for the
'characterization number.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:MIX:ECAL:CHAR 1,0"
'Specify the thru measurement method. This applies to both ECal
'and mechanical calibrations. For ECal 'DEFAULT' will use the ECal
'thru. Other choices may be used depending on the genders and types
'of the connectors on the test interface.
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:METH ""DEFAULT""
'Omit the isolation part of the 2-port cal
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:OMIT 1"
'Turn on auto orientation for the ECal
SCPI.Execute "SENS:CORR:COLL:SESS6:VMC:TWOP:ECAL:ORI:STATE 1"

'Tell the wizard to generate and report the number of steps in this
'cal session
Dim steps
Dim desc
'Determine the number of steps required to complete the calibration.
'First send the write command, then the query.
SCPI.Execute "SENS:CORR:COLL:SESS6:STEP"
steps = SCPI.Execute ("SENS:CORR:COLL:SESS6:STEP?")
For i = 1 To steps
 'Display the prompt for each step
 desc = SCPI.Execute ("SENS:CORR:COLL:SESS6:DESC? " & CStr(i))
 MsgBox (desc)
 'Perform the measurement for each step
 SCPI.Execute "SENS:CORR:COLL:SESS6:ACQ " & CStr(i)
Next
Dim calset
'Finish the cal and save the calset
calset = SCPI.Execute ("SENS:CORR:COLL:SESS6:SAVE?")
Msgbox ("VMC Cal Complete!")

```



## Create and Cal an SMC Measurement

---

This Visual Basic example creates and calibrates a scalar mixer measurement.

To run this example **without modification** you need the following:

- A Mixer setup file saved on the PNA: C:\Program Files\Agilent\Network Analyzer\Documents\Mixer\MyMixer.mxr.
- If the mixer file uses an external LO source, it must also be attached and configured.
- An ECAL module that covers the frequency range of the measurement.
- A power meter must be attached to the PNA. If this example is run in the PNA, the power meter does not need to be attached using a GPIB/USB interface.

The SCPI commands in this example are sent over a COM interface using the SCPIStringParser object. You do NOT need a GPIB connection to run this example. However, some modification is necessary to make the program run on a traditional GPIB Interface. For example, during the power meter portion of this calibration, scpi.Execute will not process a command until the power meter routine has completed. Traditional GPIB would require a serial polling technique to ensure the routine has completed before proceeding.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as SMC.vbs. Learn how to setup and run the macro.

```
Dim app
Dim scpi
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpiStringParser
'---Create a Scalar Mixer Forward Measurement
'First, delete all measurements on the channel
scpi.Execute "CALC:PAR:DEL:ALL"
'Create a forward scalar mixer measurement and configure it in
'channel 1. The first parameter is a unique
'identifying string (specified by the user) to allow subsequent
'commands to be directed at this specific measurement.
scpi.Execute "CALC:CUST:DEF ""My SC21"", ""SMC_Forward.SMC_ForwardMeas""
'For reverse measurements, use the following:
'scpi.Execute "CALC:CUST:DEF ""My SC12"", ""SMC_Reverse.SMC_ReverseMeas""
'Setup the new measurement as the 2nd trace in the active window
scpi.Execute "DISP:WIND:TRAC2:FEED ""My SC21""
'Make the new trace the active measurement
scpi.Execute "CALC:PAR:SEL ""My SC21""
'The parameters of the mixer measurement can now be configured.
'This can be done by either using the individual SENS:MIX commands
'for each of the parameters or by loading a mixer setup file. This
'example loads a mixer setup file. The path name
'for the mixer file may be loaded from other mapped drives
scpi.Execute "SENS:MIXer:Load ""C:\Program Files\Agilent\Network
Analyzer\Documents\Mixer\MyMixer.mxr""
'-----Perform A Scalar Mixer Calibration-----
'Initialize an SMC guided calibration for session number 6
scpi.Execute "SENS:CORR:COLL:SESS6:INIT ""SMC""
'Select to use an ECal for the 2-port cal portion of the procedure
'To use a mechanical kit you will have to use the following command:
'scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOPort:OPTION ""MECH""
```

```

scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOPort:OPTion ""ECAL""
'If you select the mechanical method then you also have to
'specify the connector types and the cal kits for each of the ports.
'The comments below show an example of how that is done:
'scpi.Execute "SENS:CORR:COLL:SESS6:CONN:PORT1:SEL ""APC 3.5 male""
'scpi.Execute "SENS:CORR:COLL:SESS6:CONN:PORT2:SEL ""APC 3.5 female""
'scpi.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT1:SEL ""85052D""
'scpi.Execute "SENS:CORR:COLL:SESS6:CKIT:PORT2:SEL ""85052D""
'Specify the ECal module and the ECal characterization for this
'session. FCA calibrations currently only support ECal module
'number 1. In this example the factory characterization is used
'by specifying 0 for the characterization number.
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:ECAL:CHAR 1,0"
'Specify the thru measurement method. This applies to both ECal
'and mechanical calibrations. For ECal 'DEFAULT' will use the ECal
'thru. Other choices may be used depending on the genders and types
'of the connectors on the test interface.
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOP:METH ""DEFAULT""
'Omit the isolation part of the 2-port cal
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOP:OMIT 1"
'Turn on auto orientation for the ECal
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:TWOP:ECAL:ORI:STATE 1"
'Set the Source port for the power cal to 1. If the
'measurement is an SMC Forward the valid port settings are '1' and
''BOTH' and if the measurement is an SMC Reverse, the valid port settings
'are '2' and 'BOTH'.
scpi.Execute "SENS:CORR:COLL:SESS6:SMC:PWRC:SRCP ""1""
'Tell the wizard to generate and report the number of steps in this
'cal session
Dim steps
Dim desc
'Determine the number of steps required to complete the calibration.
'First send the write command, then the query.
scpi.Execute "SENS:CORR:COLL:SESS6:STEP"
steps = scpi.Execute ("SENS:CORR:COLL:SESS6:STEP?")
For i = 1 To steps
'Display the prompt for each step
desc = scpi.Execute ("SENS:CORR:COLL:SESS6:DESC? " & CStr(i))
MsgBox (desc)
'Perform the measurement for each step
scpi.Execute "SENS:CORR:COLL:SESS6:ACQ " & CStr(i)
Next
Dim calset
'Finish the cal and save the calset
calset = scpi.Execute ("SENS:CORR:COLL:SESS6:SAVE?")
Msgbox ("SMC Cal Complete!")

```

## Create an SMC Fixed Output Measurement

---

This VB Script example creates a calibrated SMC fixed output measurement using a controlled LO. Then a single sweep is taken and data is retrieved. You can run a VBScript (\*.vbs) program from the PNA [using Macros](#).

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object.

Fixed output measurements are only supported on SMC (not VMC) measurements. Fixed output measurements require that an external LO source be sweeping and synchronized with the PNA source. FCA can perform this synchronization using the external source configuration settings.

The fastest, and recommended, method of controlling the LO source is [Hardware List \(BNC\) triggering mode](#). However, in this mode, FCA channels will not respond to manual triggers. Therefore, the example uses the following mechanism to trigger a sweep:

```
Write "SENS:SWE:MODE HOLD" 'place channel 1 in HOLD mode
Write "INIT:CONT ON" 'place PNA in internal trigger mode
Write "SENS:SWE:GRO:COUNT 1" 'specify that the group count is 1 sweep
Write "SENS:SWE:MODE GROUPS" 'execute group count (1 sweep)
Write "*OPC?" 'wait until the sweep is complete
Read
```

Both VMC and SMC measurements require that mixer parameters be setup before making the measurement. The mixer parameters are not applied until calling [SENS:MIX:CALC](#)

You can also setup the mixer parameters using [SENS:MIX:LOAD](#). With this interface, the specified mixer file is loaded and immediately applied.

To run this program, copy the following code into a text editor and save it as a \*.vbs file.

```
option explicit

' Setup infrastructure to use the SCPI over COM
dim app
set app = createobject("Agilentpna835x.application")
dim p
set p = app.scpistringparser
dim returnStr

sub Write (command)
if len(returnStr) <> 0 then
err.Raise 55,"Write","Query Unterminated"
end if
returnStr = p.parse(command)
end sub

sub WriteIgnoreError(command)
returnStr = p.Execute(command)
p.Parse("SYST:ERR?") ' clear error queue
end sub

function Read
if len(returnStr) = 0 then
err.Raise 55,"Read","Bad read"
end if
Read = returnStr
returnStr = ""
end function

Write "SYST:PRES"
```

```

' When programming in remote mode, hold mode is recommended
Write "SENS:SWE:MODE HOLD"

' Select calibration. Use execute so that errors get ignored
WriteIgnoreError "SENS:CORR:CSET:GUID '{C9080B34-EF1F-4ED5-B07D-250B45962B99}'"

' Delete the standard measurement
Write "CALC:PAR:DEL:ALL"

' Create an SC21 measurement
Write "CALC:CUST:DEF 'MySMC', 'SMC_Forward.SMC_ForwardMeas'"
Write "DISP:WIND:TRACE:FEED 'MySMC'"
Write "CALC:PAR:SEL 'MySMC'"
Write "CALC:CUST:MOD 'SC21'"

' Set number of points to 11
Write "SENS:SWE:POIN 11 "

' Setup the mixer parameters for a swept LO, fixed output measurement
Write "SENS:MIX:INP:FREQ:START 200e6"
Write "SENS:MIX:INP:FREQ:STOP 700e6"
Write "SENS:MIX:LO:FREQ:MODE Swept"
Write "SENS:MIX:OUTPUT:FREQ:FIX 3.4e9"
Write "SENS:MIX:OUTP:FREQ:SID HIGH"
Write "SENS:MIX:INP:POW -17"
Write "SENS:MIX:LO:POW 10"
' Specify the LO name, for controlled LO.
' This name is setup in the External Source Config Dialog
Write "SENS:MIX:LO:NAME '8360'"
' The CALC method calculates the LO frequency from the other parameters,
' It also applies the mixer parameters to the channel.
Write "SENS:MIX:CALC LO_1"

' Create an S11 in the same channel
Write "CALC:CUST:DEF 'MyS11', 'SMC_Forward.SMC_ForwardMeas'"
Write "DISP:WIND:TRACE2:FEED 'MyS11'"
Write "CALC:PAR:SEL 'MyS11'"
Write "CALC:CUST:MOD 'S11'"

' Create an IPwr in the same channel
Write "CALC:CUST:DEF 'MyIPwr', 'SMC_Forward.SMC_ForwardMeas'"
Write "DISP:WIND:TRACE3:FEED 'MyIPwr'"
Write "CALC:PAR:SEL 'MyIPwr'"
Write "CALC:CUST:MOD 'IPwr'"

' Create an OPwr in the same channel
Write "CALC:CUST:DEF 'MyOPwr', 'SMC_Forward.SMC_ForwardMeas'"
Write "CALC:PAR:SEL 'MyOPwr'"
Write "DISP:WIND:TRACE4:FEED 'MyOPwr'"
Write "CALC:CUST:MOD 'OPwr'"

' Perform a single sweep, synchronously. When *OPC returns, the sweep is done
Write "SENS:SWE:GRO:COUN 1"
Write "SENS:SWE:MODE GROUPS"
Write "**OPC?"
Read

```



```
' Retrieve the SC21 data
Write "CALC:PAR:SEL 'MySMC'"
Write "CALC:DATA? SDATA"
dim data
data = Read()
wscript.echo(data)

'Retrieve the S11 data
Write "CALC:PAR:SEL 'MyS11'"
Write "CALC:DATA? SDATA"
data = Read()
wscript.echo(data)
```

## Getting and Putting Data using SCPI

---

This Visual Basic Program does the following:

- Reads data from the analyzer
- Puts the data back into memory
- To see the data on the analyzer after running the program, from the front panel click:  
**Trace - Math/Memory - Memory Trace**

To run this program, you need:

- An established GPIB interface connection

### See Other SCPI Example Programs

---

**Note:** To change the read and write location of data, removing the comment from the beginning of ONE of the lines, and replace the comment in the beginning of the SDATA and SMEM lines.

---

```
Private Sub ReadWrite_Click()
Dim i As Integer
Dim t As Integer
Dim q As Integer
Dim dat As String
Dim cmd As String
Dim datum() As Double

GPIB.Configure
GPIB.Write "SYSTem:PRESet;*wai"

'Select the measurement
GPIB.Write "CALCulate:PARAmeter:SElect 'CH1_S11_1'"

'Read the number of data points
GPIB.Write "SENSel:SWEep:POIN?"
numpts = GPIB.Read

'Turn continuous sweep off
GPIB.Write "INITiate:CONTinuous OFF"

Take a sweep
GPIB.Write "INITiate:IMMediate;*wai"

'Ask for the Data

'PICK ONE OF THESE LOCATIONS TO READ
'GPIB.Write "CALCulate:DATA? FDATA" 'Formatted Meas
'GPIB.Write "CALCulate:DATA? FMEM" 'Formatted Memory
GPIB.Write "CALCulate:DATA? SDATA" 'Corrected, Complex Meas
'GPIB.Write "CALCulate:DATA? SMEM" 'Corrected, Complex Memory
'GPIB.Write "CALCulate:DATA? SCORR1" 'Error-Term Directivity

'Number of values returned per data point
'q = 1 ' Pick this if reading FDATA or FMEM
q = 2 ' Otherwise pick this

'Parse the data
ReDim datum(q, numpts)
```

```

For i = 0 To numpts - 1
 For t = 0 To q - 1
 'Read the Data
 dat = GPIB.Read(20)
 'Parse it into an array
 datum(t, i) = Val(dat)
 Next t
Next i

'PUT THE DATA BACK IN
GPIB.Write "format ascii"

'PICK ONE OF THESE LOCATIONS TO PUT THE DATA
'cmd = "CALCulate:DATA FDATA," 'Formatted Meas
'cmd = "CALCulate:DATA FMEM," 'Formatted Memory
'cmd = "CALCulate:DATA SDATA," 'Corrected, Complex Meas
cmd = "CALCulate:DATA SMEM," 'Corrected, Complex Memory
'cmd = "CALCulate:DATA SCORR1," 'Error-Term Directivity

For i = 0 To numpts - 1
 For t = 0 To q - 1
 If i = numpts - 1 And t = q - 1 Then
 cmd = cmd & Format(datum(t, i))
 Else
 cmd = cmd & Format(datum(t, i)) & ","
 End If
 Next t
Next i

GPIB.Write cmd
End Sub

```

## Getting and Putting Data

---

This Rocky Mountain Basic example does the following:

1. Takes a sweep, and reads the formatted data trace into an array. The trace is read as a definite length block.
2. Instructs you to remove DUT
3. Downloads the trace back to the analyzer as an definite length block.

### See Other SCPI Example Programs

```
100 DIM A$(10),Data1(1:51)
110 INTEGER Digits,Bytes
120 !
130 COM /Sys_state/ @Hp87xx,Scode
140 ! Identify I/O Port
150 CALL Iden_port
160 !
170 !
180 OUTPUT @Hp87xx;"SYST:PRES"
190 !
200 OUTPUT @Hp87xx;"CALC:PAR:SEL 'CH1_S11_1'"
210 !
220 ! Set up the analyzer to measure 51 data points.
230 OUTPUT @Hp87xx;"SENS1:SWE:POIN 51;*OPC?"
240 ENTER @Hp87xx;Opc
250 !
260 ! Take a single sweep, leaving the analyzer
270 ! in trigger hold mode.
280 OUTPUT @Hp87xx;"ABOR;:INIT1:CONT OFF;:INIT1;*WAI"
290 !
300 ! Select binary block transfer
310 OUTPUT @Hp87xx;"FORM:DATA REAL,64"
320 !
330 ! Request the channel 1 formatted data array
340 ! from the analyzer.
350 OUTPUT @Hp87xx;"CALC:DATA? FDATA"
360 !
370 ! Turn on ASCII formatting on the I/O path.
380 ! It is needed for reading the header
390 ! information.
400 ASSIGN @Hp87xx;FORMAT ON
410 !
420 ! Get the data header. "A$" will contain the
430 ! "#" character indicating a block data transfer.
440 ! "Digits" will contain the number of characters
450 ! for the number of bytes value which follows.
460 ENTER @Hp87xx USING "%,A,D";A$,Digits
470 !
480 ! Get the rest of the header. The number of
490 ! bytes to capture in the data array will be
```

```

500 ! placed in "Bytes". Note the use of "Digits"
510 ! in the IMAGE string.
515 !
520 ENTER @Hp87xx USING "%,"&VAL$(Digits)&"D";Bytes
525 PRINT "HEADER",A$,Digits,Bytes
530 !
540 ! Turn off ASCII formatting on the I/O path;
550 ! it is not needed for transferring binary
560 ! formatted data.
570 ASSIGN @Hp87xx;FORMAT OFF
580 !
590 ! Get the data.
600 ENTER @Hp87xx;Data1(*)
610 !
620 ! Turn on ASCII formatting again.
630 ASSIGN @Hp87xx;FORMAT ON
640 !
650 ! Get the "end of data" character.
660 ENTER @Hp87xx;A$
670 !
680 ! Display the first three numbers in the array.
690 DISP "Trace: ";Data1(1);Data1(2);Data1(3);"..."
700 !
710 ! Use this time to visually compare the
720 ! numbers to the visible data trace.
730 WAIT 5
740 !
750 ! Prompt the operator to disconnect the test
760 ! device and how to continue the program.
770 DISP "Disconnect the test device -- Press Continue"
780 PAUSE
790 !
800 ! Update the display line.
810 DISP "Taking a new sweep...";
820 !
830 ! Take a sweep so the display shows new data.
840 OUTPUT @Hp87xx;":INIT1;*WAI"
850 DISP " Done."
860 WAIT 5
870 !
880 ! Send the header for an indefinite block length
890 ! data transfer.
900 DISP "Downloading saved trace...";
915 ! The first byte '3' indicates the next three digits equal number of transfer
bytes
916 ! The number of transfer bytes equals 8x the number of tracepoints.
920 OUTPUT @Hp87xx;"CALC:DATA FDATA, #3408";
930 !
940 ! Turn off ASCII formatting.
950 ASSIGN @Hp87xx;FORMAT OFF
960 !
970 ! Send the data array back to the analyzer.
980 OUTPUT @Hp87xx;Data1(*),END
990 !
1000 ! Turn on ASCII formatting again.
1010 ASSIGN @Hp87xx;FORMAT ON
1020 DISP " Done!"

```

```

1030 END
1040 !
1050 !*****
1060 ! Iden_port: Identify io port to use
1070 ! Description: This routines sets up the I/O port address for
1080 ! the SCPI interface. For "HP 87xx" instruments,
1090 ! the address assigned to @Hp87xx = 800 otherwise,
1100 ! 716.
1110 !*****
1120 SUB Iden_port
1130 COM /Sys_state/ @Hp87xx,Scode
1140 !
1150 IF POS(SYSTEM$("SYSTEM ID"),"HP 87")<>0 THEN
1160 ASSIGN @Hp87xx TO 800
1170 Scode=8
1180 ELSE
1190 ASSIGN @Hp87xx TO 716
1200 Scode=7
1210 END IF
1220 !
1230 SUBEND !Iden_port
1240 !

```

## Transfer Data using GPIB

---

The following RMB examples transfer data to and from a remote PC using the MMEM:TRANsfer command.

### Transferring data FROM the PNA -- TO a remote PC:

```
30 !
40 ! Set up I/O paths
50 !
60 ! Network analyzer address
70 ASSIGN @Na TO 716
75 !
77 ! File to be stored on local computer
80 ! First time -- need to create the file.
90 ! After file name, number records set to 0 (ignored by WinOS)
95 ! Use "PURGE" command to delete if desired.
100 CREATE "mytestdata.s2p",0
110 ASSIGN @File TO "mytestdata.s2p"
120 !
122 ! TRANSFER the data (download)
123 !
125 ! Analyzer has file 'testdata.s2p' in default directory
130 OUTPUT @Na;" :MMEM:TRAN? "testdata.s2p""
135 !
137 ! Now unravel the bytes coming back from the analyzer.
140 ENTER @Na USING "#,A";A$
150 ENTER @Na USING "#,A";Digit$
160 !
170 ! Create appropriate "image"
180 Img$="#",&Digit$&"A"
190 !
200 ! Byte$ holds the number of bytes in string format
210 ENTER @Na USING Img$;Byte$
220 !
230 ! Allocate a buffer for holding the data
240 ALLOCATE Dat$[VAL(Byte$)]
250 !
260 ! Set up a different image for filling the buffer
270 Img$=Byte$&"A"
280 !
290 ! Retrieve the actual file data
300 ENTER @Na USING Img$;Dat$
305 !
307 ! Now save the file locally.
310 OUTPUT @File;Dat$
320 END
```

### Transferring data FROM the remote PC - TO the PNA:

```
40 ! Set up I/O paths
50 !
60 ! Network analyzer address
70 ASSIGN @Na TO 716
77 ! File to be retrieved from local computer
78 ASSIGN @File TO "mytestdata.s2p"
```

```
79 !
120 !
122 ! TRANSFER the data
123 !
230 ! Allocate a buffer for holding the data
240 ALLOCATE Dat$(26236)
250 !
260 ! Get data from the file and fill Dat$
270 ENTER @File;Dat$
280 !
325 ! Data to be transferred to analyzer file 'testupld.s2p'
325 ! in default directory.
326 !
327 ! A specific block transfer designator must follow the
328 ! file name:
329 ! '#' specifies a block transfer.
330 ! '6' specifies 6 digits to follow.
331 ! '026236' matches the buffer size allocated above
332 ! not counting <NL><END> (new line and end of file).
430 OUTPUT @Na;":MMEM:TRAN ""testupld.s2p",#6026236",Dat$
520 END
```



## Establish a VISA Session

---

This Visual Basic program demonstrates how to send a SCPI command using VISA and the Agilent IO libraries. To run this program, you need:

- Your PC and PNA both connected to a LAN (for communicating with each other).
- The SICL and VISA components of Agilent's I/O Libraries software installed on your PC. Both are included when you install the software, unless you already have another vendor's VISA installed. Then specify Full SICL and VISA installation to overwrite the other vendor's VISA.
- The module visa32.bas added to your VB project. After you install VISA, the module will be located at C:\VXI\PNP\WINNT (or equivalent)\INCLUDE\Visa32.bas
- A form with two buttons: cmdRun and cmdQuit.
- Your PC configured to be a VISA LAN Client, and the SICL Server capability enabled on the PNA. See [Configure for VISA and SICL](#)

---

### See Other SCPI Example Programs

**Note:** This example is a piece of a larger VISA program that performs a source power calibration.

---

```
'Session to VISA Default Resource Manager
Private defRM As Long
'Session to PNA
Private viPNA As Long
'VISA function status return code
Private status As Long

Private Sub Form_Load()
defRM = 0
End Sub

Private Sub cmdRun_Click()
' String to receive data from the PNA.
' Dimensioned large enough to receive scalar comma-delimited values
' for 21 frequency points (20 ASCII characters per point)
Dim strReply As String * 420

' Open the VISA default resource manager
status = viOpenDefaultRM(defRM)
If (status < VI_SUCCESS) Then HandleVISAError

' Open a VISA session (viPNA) to the SICL LAN server
' at "address 16" on the PNA pointed to by the "GPIB0"
' VISA LAN Client on this PC.
' CHANGE GPIB0 TO WHATEVER YOU PNA IS SET TO
status = viOpen(defRM, "GPIB0::16::INSTR", 0, 0, viPNA)
If (status < VI_SUCCESS) Then HandleVISAError

' Need to set the VISA timeout value to give all our calls to
' myGPIBRead sufficient time to complete before a timeout
' error occurs.
' For this example, let's try setting the limit to
' 30000 milliseconds (30 seconds).
status = viSetAttribute(viPNA, VI_ATTR_TMO_VALUE, 30000)
```

```

If (status < VI_SUCCESS) Then HandleVISAError

' Preset the PNA
status = myGPIBWrite(viPNA, "SYST:PRES")
If (status < VI_SUCCESS) Then HandleVISAError

' Print the data using a message box
MsgBox strReply
End Sub

Private Sub cmdQuit_Click()
' Close the resource manager session (which also closes
' the session to the PNA).
If defRM <> 0 Then Call viClose(defRM)

' End the program
End
End Sub

Private Function myGPIBWrite(ByVal viHandle As Long, ByVal strOut As String) As Long
' The "+ Chr$(10)" appends an ASCII linefeed character to the
' output, for terminating the write transaction.
myGPIBWrite = viVPrintf(viHandle, strOut + Chr$(10), 0)
End Function

Private Function myGPIBRead(ByVal viHandle As Long, strIn As String) As Long
myGPIBRead = viVScanf(viHandle, "%t", strIn)
End Function

Sub HandleVISAError()
Dim strVisaErr As String * 200
Call viStatusDesc(defRM, status, strVisaErr)
MsgBox "*** Error : " + strVisaErr, vbExclamation
End
End Sub

```

[See Other SCPI Example Programs](#)

## Status Reporting using SCPI

---

This Visual Basic program demonstrates two methods of reading the analyzer's status registers:

- Polled Bit Method - reads the Limit1 register continuously.
- SRQ Method - enables an interrupt of the program when bit 6 of the status byte is set to 1. The program then queries registers to determine if the limit line failed.

To run this program, you need:

- An established [GPIB interface connection](#)
- A form with two buttons: Poll and SRQ Method
- A means of causing the limit line to fail, assuming it passes initially.

```
Private Sub Poll_Click()
' POLL THE BIT METHOD
' Clear status registers
GPIB.Write "*CLS"

'Loop FOREVER
Do
 DoEvents
 GPIB.Write "STATus:QUESTionable:LIMit1:EVENT?"
 onn = GPIB.Read
Loop Until onn = 2

MsgBox "Limit 1 Failed "
End Sub

Private Sub SRQMethod_Click()
'SRQ METHOD
GPIB.Write "SYSTem:PRESet"
GPIB.Write "CALCulate:PARAMeter:SElect 'CH1_S11_1'"
↑ low down the trace
GPIB.Write "SENS:BWID 150"

'Setup limit line
GPIB.Write "CALC:LIM:DATA 2,3e9,6e9,-2,-2"
GPIB.Write "CALC:LIMit:DISP ON"
GPIB.Write "CALC:LIMit:STATe ON"

' Clear status registers.
GPIB.Write "*CLS;*wai"
' Clear the Service Request Enable register.
GPIB.Write "**SRE 0"
' Clear the Standard Event Status Enable register.
GPIB.Write "**ESE 0"

' Enable questionable register, bit(10) to report to the status byte.
GPIB.Write "STATus:QUESTionable:ENABle 1024"
```

```

' Enable the status byte register bit3 (weight 8) to notify controller
 GPIB.Write "*SRE 8"

' Enable the onGPIBNotify event
 GPIB.NotifyMask = cwGPIBRQS
 GPIB.Notify
End Sub

Private Sub GPIB_OnGPIBNotify(ByVal mask As Integer)
' check to see what failed
' was it the analyzer?
 GPIB.Write "*STB?"
onn = GPIB.Read
If onn <> 0 Then
' If yes, then was it the questionable register?
 GPIB.Write "STATus:QUESTIONable:EVENT?"
onn = GPIB.Read
' Determine if the limit1 register, bit 8 is set.
If onn = 1024 Then
'if yes, then was it trace 1?
 GPIB.Write "STAT:QUES:LIMIT1:EVENT?"
onn = GPIB.Read
If onn = 2 Then MsgBox ("Limit Line1 Failed")
End If
End If
End Sub

```

## GPIB using Visual C++

---

### See Other SCPI Example Programs

```
/*
 * This example assumes the user's PC has a National Instruments GPIB board. The
example is comprised of three basic parts:
 *
 * 1. Initialization
 * 2. Main Body
 * 3. Cleanup
 *
 * The Initialization portion consists of getting a handle to the PNA and then doing
a GPIB clear of the PNA.
 *
 * The Main Body consists of the PNA SCPI example.
 *
 * The last step, Cleanup, releases the PNA for front panel control.
 */

#include <stdio.h>
#include <stdlib.h>

/*
 * Include the WINDOWS.H and DECL-32.H files. The standard Windows
 * header file, WINDOWS.H, contains definitions used by DECL-32.H and
 * DECL-32.H contains prototypes for the NI GPIB routines and constants.
 */
#include <windows.h>
#include "decl-32.h"

#define ERRMSGSIZE 1024 // Maximum size of SCPI command string
#define ARRAYSIZE 1024 // Size of read buffer

#define BDINDEX 0 // Board Index of GPIB board
#define PRIMARY_ADDR_OF_PNA 16 // GPIB address of PNA
#define NO_SECONDARY_ADDR 0 // PNA has no Secondary address
#define TIMEOUT T10s // Timeout value = 10 seconds
#define EOTMODE 1 // Enable the END message
#define EOSMODE 0 // Disable the EOS mode

int pna;
char ValueStr[ARRAYSIZE + 1];
char ErrorMnemonic[21][5] = {"EDVR", "ECIC", "ENOL", "EADR", "EARG",
 "ESAC", "EABO", "ENEB", "EDMA", "",
 "EOIP", "ECAP", "EFSO", "", "EBUS",
 "ESTB", "ESRQ", "", "", "", "ETAB"};

void GPIBWrite(char* SCPIcmd);
char *GPIBRead(void);
void GPIBCleanup(int Dev, char* ErrorMessage);

int main()
{
```

```

char *opc;
char *result;
char *value;

/*
 * =====
 * INITIALIZATION SECTION
 * =====
 */

/*
 * The application brings the PNA online using ibdev. A device handle,pna, is
returned and is used in all subsequent calls to the PNA.
 */
pna = ibdev(BDINDEX, PRIMARY_ADDR_OF_PNA, NO_SECONDARY_ADDR,
TIMEOUT, EOTMODE, EOSMODE);
if (ibsta & ERR)
{
printf("Unable to open handle to PNA\nibsta = 0x%x iberr = %d\n",
ibsta, iberr);
return 1;
}

/*
 * Do a GPIB Clear of the PNA. If the error bit ERR is set in ibsta, call
GPIBCleanup with an error message.
 */
ibclr (pna);
if (ibsta & ERR)
{
GPIBCleanup(pna, "Unable to perform GPIB clear of the PNA");
return 1;
}

/*
 * =====
 * MAIN BODY SECTION
 * =====
 */

// Reset the analyzer to instrument preset
GPIBWrite("SYSTem:FPRESET");

// Create S11 measurement
GPIBWrite("CALCulatel:PARAMeter:DEFine 'My_S11',S11");

// Turn on Window #1
GPIBWrite("DISPlay:WINDow1:STATe ON");

// Put a trace (Trace #1) into Window #1 and 'feed' it from the measurement
GPIBWrite("DISPlay:WINDow1:TRACel:FEED 'My_S11'");

// Setup the channel for single sweep trigger
GPIBWrite("INITiatel:CONTinuous OFF;*OPC?");
opc = GPIBRead();
GPIBWrite("SENSel:SWEep:TRIGger:POINT OFF");

```

```

// Set channel parameters
GPIBWrite("SENSE1:SWEep:POINTs 11");
GPIBWrite("SENSE1:FREQuency:START 1000000000");
GPIBWrite("SENSE1:FREQuency:STOP 2000000000");

// Send a trigger to initiate a single sweep
GPIBWrite("INITiate1;*OPC?");
opc = GPIBRead();

// Must select the measurement before we can read the data
GPIBWrite("CALCulate1:PARAMeter:SElect 'My_S11'");

// Read the measurement data into the "result" string variable
GPIBWrite("FORMat ASCII");
GPIBWrite("CALCulate1:DATA? FDATA");
result = GPIBRead();

// Print the data to the display console window
printf("S11(dB) - Visual C++ SCPI Example for PNA\n\n");
value = strtok(result, ",");
while (value != NULL)
{
printf("%s\n", value);
value = strtok(NULL, ",");
}

/*
* =====
* CLEANUP SECTION
* =====
*/

/* The PNA is returned to front panel control. */
ibonl(pna, 0);

return 0;
}

/*
* Write to the PNA
*/
void GPIBWrite(char* SCPIcmd)
{
int length;
char ErrorMessage[ERRMSGSIZE + 1];
length = strlen(SCPIcmd) ;

ibwrt (pna, SCPIcmd, length);
if (ibsta & ERR)
{
strcpy(ErrorMessage, "Unable to write this command to PNA:\n");
strcat(ErrorMessage, SCPIcmd);

GPIBCleanup(pna, ErrorMessage);
exit(1);
}
}

```

```

}

/*
 * Read from the PNA
 */
char* GPIBRead(void)
{
 ibrd (pna, ValueStr, ARRAYSIZE);
 if (ibsta & ERR)
 {
 GPIBCleanup(pna, "Unable to read from the PNA");
 exit(1);
 }
else
 return ValueStr;
}

/*
 * After each GPIB call, the application checks whether the call succeeded. If an
NI-488.2 call fails, the GPIB driver sets the corresponding bit in the global status
variable. If the call failed, this procedure prints an error message, takes the PNA
offline and exits.
 */
void GPIBCleanup(int Dev, char* ErrorMessage)
{
 printf("Error : %s\nibsta = 0x%x iberr = %d (%s)\n",
 ErrorMessage, ibsta, iberr, ErrorMnemonic[iberr]);
 if (Dev != -1)
 {
 printf("Cleanup: Returning PNA to front panel control\n");
 ibonl (Dev, 0);
 }
}
}

```



## Create a Custom Power Meter Driver

---

**Note:** This topic requires that you have a working knowledge of Visual Basic.

---

This topic will help you create your own power meter driver for use with Source Power Calibration on the PNA. If you are using one of the following Power Meters to perform a Source Power Calibration, you do NOT need to create your own driver:

E4416A, E4417A, E4418A/B, E4419A/B, 437B, 438A, EPM-441A, EPM-442A

Your Power Meter driver will be created from a template written in Visual Basic using VISA over the GPIB bus.

**Note:** This procedure applies to Visual Basic 6.0. Applicability to Visual Basic .NET has not yet been investigated.

---

### Prepare Template Files

### Modify Template Files

### Compile, Copy, and Register, Your New Driver

### Test Your new Driver

## Other SCPI Example Programs

---

### Prepare Template Files

1. Copy all the files from the PNA hard drive C:\Program Files\Agilent\Network Analyzer\Automation\Power Meter Driver Template folder, to a folder on your development PC.
2. In Visual Basic click **File**, then **Open Project...**, find **MyPowerMeter.vbp** (a file you copied from the PNA). Click **Open**. This is a VB ActiveX EXE template, which you will fill in to become your driver.
3. Click **Project**, then **MyPowerMeter Properties**. Click the **General** tab.
4. Overwrite the Project Name with a name of your own choosing. This will be the name of your driver's type library (also the default name of your exe).



**Note** If the name of your exe does not match the VB Project Name with which it was compiled, registration of the exe on the PNA will not succeed.

---

5. Set the Project Description. After building your driver if you wish to test it using VB, this is the string that will show up in the VB References list of your test project, and also in the lower pane of the VB Object Browser.
6. Set the Thread Pool size to 1 thread.
7. Click **OK** to close the project properties dialog.
8. From the VB **Project** menu, click **References...** Ensure that **Agilent PNA Power Meter 1.0 Type Library** and **VISA Library** are checked. Click **OK**.

**Note:** Agilent's implementation of VISA is installed as part of the Agilent I/O Libraries on the PNA. For help on VISA, go to the Windows Start button on your PNA, select Programs, Agilent IO Libraries, VISA Help.

---

## Modify Template Files

From Visual Basic **View** menu click **Project Explorer**. Expand the **Modules** and **Class Modules** folders. Ensure there is one module (WinAPI) and one class module (PowerMeter).

Let's look at the WinAPI module first.

1. In the **Project Explorer** window, click **WinAPI**.
2. From the **View** menu click **Code**.

There is only one line of code you should need to modify in this module: the value of the string constant named `sIDSEARCH`. The comments preceding the declaration of that string describe how to change it. The rest of this module contains functions which will use the Microsoft Windows API to insure proper registration of your driver on the PNA. If you know of other Windows API functions you feel might be helpful to call from within your PowerMeter class module (to help in formatting data, for example), this module would be the place to declare them.

Now let's look at the class module.

1. In the Project Explorer window, click **PowerMeter**.
2. From the **View** menu click **Properties Window**. The **Instancing** property must be set to MultiUse. This allows other applications to create objects from this class, such that one instance of your driver EXE can supply more than one such object at a time.
3. From the **View** menu click **Code**.

Do NOT modify the Interfaces to IPowerMeter subroutines and functions. PNA source power cal expects to find these interfaces as they are currently defined.

The only members that you need to supply code to are those containing “**Your code here**” comments.

In addition, comments have been provided at the beginning of each member to describe the information that member needs to be read from or written to the power meter.

To get an idea of how communicate with the power meter using the VISA functions **viWrite** and **viRead**, examine the code which has been implemented for you in `IPowerMeter_Connect`, `IPowerMeter_QueryMeter`, and `IPowerMeter_WriteMeter`.

---

## Compile, Copy, and Register Your New Driver

When your driver is ready to run, you will first need to compile it into an EXE.

From the File menu select **Make exe**.

After compiling, the following will instruct VB to use the same ID (GUID) every time you re-compile your project.

1. From the **Project** menu, click **PowerMeter Properties**.
2. On the **Component** tab, select **Binary Compatibility** and click ...
3. Browse to and select your project EXE. Click **Open**.
4. Click **OK** to close **Project Properties**.
5. Save your project.
6. Copy your driver EXE file to a folder on your PNA (do NOT use C:\Program Files\Agilent\Network Analyzer\Automation\Power Meter Driver Template folder).

7. Run the EXE file. A message box will pop up reporting whether or not registration was successful. If not successful, it will make a suggestion on what to fix.

When your driver is properly registered, PNA Source Power Cal should be able to associate it with the ID string of your power meter.

---

### Test Your Power Meter Driver

We have also provided a Visual Basic project to test your new Power Meter driver. This project individually calls every IPowerMeter method and property in your driver to verify that it performs correctly. Before running the test your PC and PNA must be configured to communicate using DCOM.

1. Connect your PC and the PNA to LAN.
2. Add your PC logon to the PNA. Both logons and password must match to communicate using DCOM. See [Additional PNA users](#).
3. Configure your driver using DCOM Config on the PNA. This will give you permission to launch and access the driver. See [Configure for COM-DCOM Programming](#).

### Modify the Test Project

1. In Visual Basic click **File**, then **Open Project...**, find **MyPowerMeterTest.vbp** (a file you copied from the PNA). Click **Open**.
2. From the **Project** menu, click **References...** From the list, find and check your new Power Meter Driver. (It should have been registered on your PC when you successfully made your driver EXE.) Click **OK**.
3. From the **View** menu click **Code**.
4. Modify the **CreateObject** line as follows:  
Replace **MyPowerMeter** with the Project Name that you chose for your driver  
Replace **MyPNA** with the Computer Name of your PNA.  
For example:

```
Set PowerMeterObj = CreateObject("AcmeBrand.PowerMeter", "AGILENT-PNA123")
```

(This assumes that you kept **PowerMeter** as class module name in your driver.)

### Run the Test Project

Ensure your power meter is connected to the PNA with a GPIB cable.

Put the PNA in system controller mode:

1. From the PNA **System** menu point to **Configure** then click **SICL/GPIB**.
2. In the GPIB box click **System Controller**.

Run the test project. If there are no errors, the driver is created successfully. If there are errors, try to figure out what went wrong and fix it. Then re-compile, re-copy the .exe to the PNA, and re-run the test. You should not need to re-register the driver or re-modify the test program.

## GPIB Pass-Through Example

---

The SCPI `SYSTem` commands used in this example allow you to send GPIB commands to another GPIB device through the PNA. The other GPIB device cannot be connected to the GPIB bus through the PNA rear panel if the PNA is being controlled by a remote PC using that connector. The other device would typically be connected to the PNA using a [USB/GPIB interface](#).

This VB Script example uses the COM `SCPIStringParser` object. However, this is not critical to the use of these commands; they can be sent using the normal syntax of your programming environment. Using the `SCPIStringParser` over LAN allows you to communicate with GPIB devices without requiring your remote PC to have a GPIB interface card installed.

Although this method of pass-through works for most applications, there are a couple of limitations:

- All data is transferred using ASCII format. Therefore, transferring large blocks of data is very slow.
- Only read and write functions are possible. Service Interrupts are not supported.

### See Other SCPI Example Programs

---

```
option explicit
dim app
set app = CreateObject("AgilentPNA835x.Application")

dim p
set p = app.ScpiStringParser

' Open a new GPIB session on Bus:2 Device:14 Timeout: 100ms
p.Parse "SYST:COMM:GPIB:RDEV:OPEN 2,14,100"
dim handleAsStr

' Retrieve the handle (ID number)
handleAsStr = p.Parse ("SYST:COMM:GPIB:RDEV:OPEN?")

' Convert the handle to an integer
dim handleAsInt
handleAsInt = CInt(handleAsStr)

' Send the "*IDN?" query
p.Parse "SYST:COMM:GPIB:RDEV:WRITE " & handleAsInt & ", '*IDN?'"

' Read its results
dim idn
idn = p.Parse("SYST:COMM:GPIB:RDEV:READ? " & handleAsInt)
msgbox idn

' Close the GPIB session
p.Parse "SYST:COMM:GPIB:RDEV:CLOSE " & handleAsInt
```

## PNA as Controller and Talker / Listener

---

This Visual Basic Program uses VISA to do the following:

- Control the PNA using a VISA LAN Client interface on the PNA.
- Control another instrument using the PNA as GPIB controller.
- Queries both the analyzer and other instrument to identify themselves with \*IDN?

---

**Note:** This program can be modified to work from a remote PC to control both instruments. In that case, set up the PNA to be a talker/listener.

---

To run this program, you need to do the following:


- Add module **visa32.bas** to the VB project. It is located on the analyzer at C:\Program Files\HP\VXIPNP\WINNT\Include\VISA32.bas
- Configure the PNA for VISA / SICL
- Set up the PNA to be GPIB system controller.
  1. On the **System** menu, point to **Configure**. Click **SICL / GPIB**
  2. Click **System Controller**
- Connect another instrument to the analyzer through a GPIB cable with Primary address of 13 on GPIB0 interface

---

### See Other SCPI Example Programs

---

```
Sub main()

'This application run from onboard the PNA
'can control both the PNA and another GPIB instrument.
'
'To run this program the module visa32.bas must be added
'to the project.

'VISA function status return code
Dim status As Long
'Session to Default Resource Manager
Dim defRM As Long
'Session to instrument
Dim viPNA As Long
'Session to other GPIB instrument
Dim viInstrument As Long
'String to hold results
Dim strRes As String * 200
On Error GoTo ErrorHandler

status = viOpenDefaultRM(defRM)
If (status < VI_SUCCESS) Then GoTo VisaErrorHandler

'Open the session to the PNA
```

```

status = viOpen(defRM, "GPIB1::16::INSTR", 0, 0, viPNA)
If (status < VI_SUCCESS) Then GoTo VisaErrorHandler

'Ask for the PNA's ID.
status = viVPrintf(viPNA, "*IDN?" + Chr$(10), 0)
If (status < VI_SUCCESS) Then GoTo VisaErrorHandler

'Read the ID as a string.
status = viVScanf(viPNA, "%t", strRes)
If (status < VI_SUCCESS) Then GoTo VisaErrorHandler
'Display the results
MsgBox "PNA is: " + strRes

'Open the session to the other instrument
status = viOpen(defRM, "GPIB0::13::INSTR", 0, 0, viInstrument)
If (status < VI_SUCCESS) Then GoTo VisaErrorHandler

'Ask for the instrument's ID.
status = viVPrintf(viInstrument, "*IDN?" + Chr$(10), 0)
If (status < VI_SUCCESS) Then GoTo VisaErrorHandler

'Read the ID as a string.
status = viVScanf(viPNA, "%t", strRes)
If (status < VI_SUCCESS) Then GoTo VisaErrorHandler

'Display the results
MsgBox "Other instrument is: " + strRes
' Close the resource manager session (which closes everything)
Call viClose(defRM)
End

ErrorHandler:
'Display the error message
MsgBox "**** Error : " + Error$, MB_ICONEXCLAMATION
End

VisaErrorHandler:
Dim strVisaErr As String * 200
Call viStatusDesc(defRM, status, strVisaErr)
MsgBox "**** Error : " + strVisaErr

End
End Sub

```

## GPIB Fundamentals

---

The General Purpose Interface Bus (GPIB) is a system of hardware and software that allows you to control test equipment to make measurements quickly and accurately. This topic contains the following information:

### [The GPIB Hardware Components](#)

### [The GPIB / SCPI Programming Elements](#)

### [How to Configure for GPIB / SICL](#)

### [SICL- RMT Operation Label](#)

### [Specifications](#)

### [GPIB Interface Capability Codes](#)

---

**Note:** All of the topics related to programming assume that you already know how to program, preferably using a language that can control instruments.

---

## Other Topics about GPIB Concepts

### The GPIB Hardware Components

The system bus and its associated interface operations are defined by the IEEE 488 standard. The following sections list and describe the main pieces of hardware in a GPIB system:

#### Instruments

The analyzer is configured as a Talker / Listener by default.

- **Talkers** are instruments that can be addressed to send data to the controller.
- **Listeners** are instruments that can be addressed to receive a command, and then respond to the command. All devices on the bus are required to listen.

#### GPIB Addresses

Every GPIB instrument must have its own unique address on the bus. The analyzer address (716) consists of two parts:

1. **The Interface select code** (typically 7) indicates which GPIB port in the system controller is used to communicate with the device.
2. **The primary address** (16) is set at the factory. You can change the primary address of any device on the bus to any number between 0 and 30. To change the analyzer address click **System \ Configure \ SICL- GPIB**

**The secondary address** is sometimes used to allow access to individual modules in a modular instrument system, such as a VXI mainframe. The analyzer does not have secondary addresses.

#### Controllers

Controllers specify the instruments that will be the talker and listener in a data exchange. The controller of the bus must have a GPIB interface card to communicate on the GPIB.

- The **Active Controller** is the computer or instrument that is currently controlling data exchanges.

- The **System Controller** is the only computer or instrument that can take control and give up control of the GPIB to another computer or instrument, which is then called the active controller.

The PNA can NOT be passed control of the GPIB. However, you can communicate with other GPIB devices through the PNA using one of, or a combination of, the following methods:

- Use the SCPI SYST:COMM:GPIB:RDEV: commands.
- Use VISA or SICL over LAN to accomplish this. See an example.
- Use USB / GPIB Interface

## Cables

GPIB Cables are the physical link connecting all of the devices on the bus. There are eight data lines in a GPIB cable that send data from one device to another. There are also eight control lines that manage traffic on the data lines and control other interface operations.

You can connect instruments to the controller in any arrangement with the following limitations:

- Do not connect more than 15 devices on any GPIB system. This number can be extended with the use of a bus extension.
- Do not exceed a total of 20 meters of total cable length or 2 meters per device, whichever is less.
- Avoid stacking more than three connectors on the back panel of an instrument. This can cause unnecessary strain on the rear-panel connector.

## The GPIB / SCPI Programming Elements

The following software programming elements combine to become a GPIB program:

### GPIB / SCPI Commands

### Programming Statements

### Instrument Drivers

## GPIB Commands

The GPIB command is the basic unit of communication in a GPIB system. The analyzer responds to three types of GPIB commands:

### 1. IEEE 488.1 Bus-management Commands

These commands are used primarily to tell some or all of the devices on the bus to perform certain interface operations.

All of the functions that can be accomplished with these commands can also be done with IEEE 488.2 or SCPI commands. Therefore, these commands are not documented in this Help system. For a complete list of IEEE 488.1 commands refer to the IEEE 488 standard. **Examples** of IEEE 488.1 Commands

- **CLEAR** - Clears the bus of any pending operations
- **LOCAL** - Returns instruments to local operation

### 2. IEEE 488.2 Common Commands



These commands are sent to instruments to perform interface operations. An IEEE 488.2 common command consists of a single mnemonic and is preceded by an asterisk ( \* ). Some of the commands have a query form which adds a "?" after the command. These commands ask the instrument for the current setting. See a complete list of the [Common Commands](#) that are recognized by the analyzer. **Examples** of IEEE 488.2 Common Commands

- `*OPC - Operation Complete`
- `*RST - Reset`
- `*OPT? - Queries the option configuration`

### 3. SCPI Commands

The Standard Commands for Programmable Instruments (SCPI) is a set of commands developed in 1990. The standardization provided in SCPI commands helps ensure that programs written for a particular SCPI instrument are easily adapted to work with a similar SCPI instrument. SCPI commands tell instruments to do device specific functions. For example, SCPI commands could tell an instrument to make a measurement and output data to a controller. **Examples** of SCPI Commands:

```
CALCULATE:AVERAGE:STATE ON
```

```
SENSE:FREQUENCY:START?
```

For more information on SCPI:

- [The Rules and Syntax of SCPI Commands](#) provides more detail of the SCPI command structure.
- [SCPI Command Tree](#) is a complete list of the SCPI commands for the analyzer

### Programming Statements

SCPI commands are included with the language specific I/O statements to form program statements. The programming language determines the syntax of the programming statements. SCPI programs can be written in a variety of programming languages such as VEE, HP BASIC, or C++. **Example** of a Visual Basic statement:


- `GPIB.Write "SOURCE:FREQUENCY:FIXED 1000 MHz"`

### Note about examples


### Instrument Drivers

Instrument drivers are subroutines that provide routine functionality and can be reused from program to program. GPIB industry leaders have written standards for use by programmers who develop drivers. When programmers write drivers that comply with the standards, the drivers can be used with predictable results. To comply with the standard, each instrument driver must include documentation describing its functionality and how it should be implemented.

**How to configure for SICL / GPIB Operation**

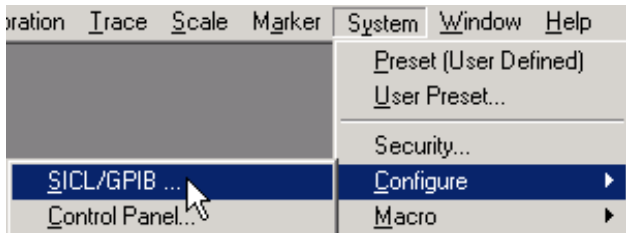

The screenshot shows a software interface with a menu bar containing 'Operation', 'Trace', 'Scale', 'Marker', 'System', 'Window', and 'Help'. The 'System' menu is open, displaying options: 'Preset (User Defined)', 'User Preset...', 'Security...', 'SICL/GPIB ...' (highlighted with a mouse cursor), and 'Control Panel...'. The 'SICL/GPIB ...' option has a right-pointing arrow next to it. Below the screenshot, there is a link: 'Learn more about using the [front panel interface](#)'.

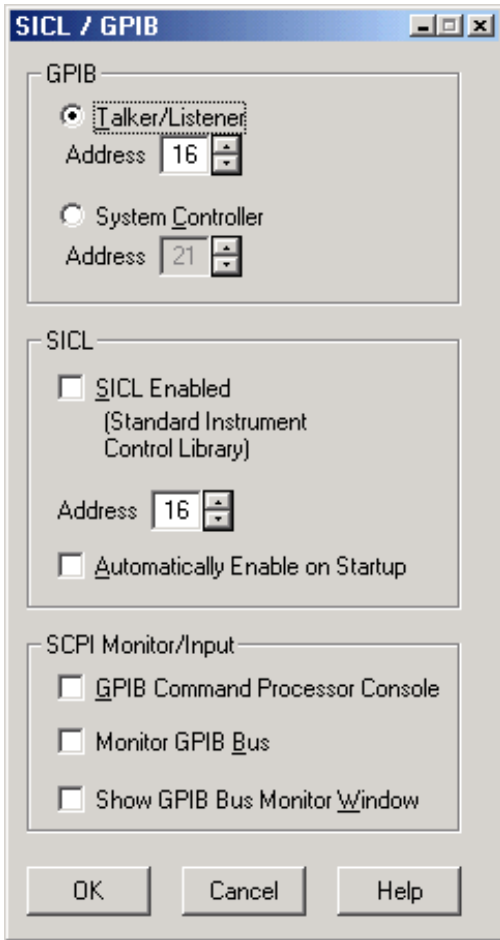

## SICL / GPIB dialog box help

### GPIB

**Talker/Listener** Sets the PNA to receive and send GPIB/SCPI messages to the system controller (external computer).

**Talker/Listener Address** Sets the PNA talker/listener GPIB address.

**System Controller** Sets the PNA as the system controller, controlling GPIB communications of external devices. Learn about the [PNA as controller](#).

**System Controller Address** Sets the PNA system controller GPIB address.

### SICL

**SICL Enabled** When checked, the analyzer is capable of running GPIB programs on its computer to control analyzer functions. The programs must be run from a GPIB-capable programming environment (VEE, Visual Basic). This mode does not allow control of external GPIB instruments. To uncheck this box, exit the PNA application - (Click File, then Exit). The PNA restarts with the SICL enabled box unchecked unless **Automatically Enable on Startup** is checked.

Learn more about [Configuring for VISA and SICL](#).

**Address** Sets the PNA address.

**Automatically Enable on Startup** When checked, SICL Enabled is automatically selected when starting the PNA application.

### SCPI Monitor / Input

**GPIB Command Processor Console** Launches a window that is used to send single SCPI/GPIB

commands.

---

**Note:** Press **Control+Z** , then enter, to close the console window.

---

- Type a valid command, with appropriate arguments and press enter.
- Use the arrow keys to recall previous commands.
- The console window may launch behind the PNA application. Press **Control+Tab** to bring the console window to the top.

**Monitor GPIB Bus** Enables monitoring activity on the GPIB.

**Show GPIB Bus Monitor Window** Shows and hides the window monitoring GPIB activity.

## LCL and RMT Operation

The analyzer **LCL** and **RMT** (Local and Remote) operation labels appear in the lower right corner of the status bar.

---

**Note:** The status bar is NOT visible when the analyzer is preset. To make the bar visible, click **View** then **Status Bar**

---

- **LCL** appears when not under SCPI control
- **RMT** appears when under SCPI control. The RMT label does NOT appear when under COM control

RMT disables the front panel keys except for the **Macro/Local** key.



Pressing the Macro / Local key returns the analyzer to Local (front panel) operation.

The IEEE488.1 "GTL" (go to local) command also returns the analyzer to Local (front panel) operation.

The IEEE488.1 "LLO" (local lockout) command disables the front panel Local button.

## GPIB Specifications

**Interconnected devices** - Up to 15 devices (maximum) on one contiguous bus.

**Interconnection path** - Star or linear (or mixed) bus network, up to 20 meters total transmission path length or 2 meters per device, whichever is less.

**Message transfer scheme** - Byte-serial, bit-parallel, asynchronous data transfer using an interlocking 3-wire handshake.

**Maximum data rate** - 1 megabyte per second over limited distances, 250 to 500 kilobytes per second typical maximum over a full transmission path. The devices on the bus determine the actual data rate.

**Address capability** - Primary addresses, 31 Talk and 31 Listen; secondary addresses, 961 Talk and 961 Listen. There can be a maximum of 1 Talker and up to 14 Listeners at a time on a single bus. See also previous section on [GPIB addresses](#).

## GPIB Interface Capability Codes

The IEEE 488.1 standard requires that all GPIB compatible instruments display their interface capabilities on the rear panel using codes. The codes on the analyzer, and their related descriptions, are listed below:

SH1 full source handshake capability

AH1 full acceptor handshake capability

T6 basic talker, serial poll, no talk only, unaddress if MLA (My Listen Address)

TEO no extended talker capability

L4 basic listener, no listen only, unaddress if MTA (My Talk Address)

LEO no extended listener capability

SR1 full service request capability

RL1 full remote / local capability

**PPO no parallel poll capability**

DC1 full device clear capability

DT1 full device trigger capability

C1 system controller capability

C2 send IFC (Interface Clear) and take charge controller capability

C3 send REN (Remote Enable) controller capability

C4 respond to SRQ (Service Request)

## The Rules and Syntax of SCPI

---

Most of the commands used for controlling instruments on the GPIB are SCPI commands. The following sections will help you learn to use SCPI commands in your programs.

### [Branches on the Command Tree](#)

### [Command and Query](#)

### [Multiple Commands](#)

### [Command Abbreviation](#)

### [Bracketed \(Optional\) Keywords](#)

### [Vertical Bars \(Pipes\)](#)


### [MIN and MAX Parameters](#)

## Other Topics about GPIB Concepts

### Branches on the Command Tree

All major functions on the analyzer are assigned keywords which are called ROOT commands. (See GPIB Command Finder for a list of SCPI root commands). Under these root commands are branches that contain one or more keywords. The branching continues until each analyzer function is assigned to a branch. A root command and the branches below it is sometimes known as a subsystem.

For example, the following graphic shows the **SOURCE** subsystem. Under the **SOURCE** and **POWER** keywords are several branch commands.

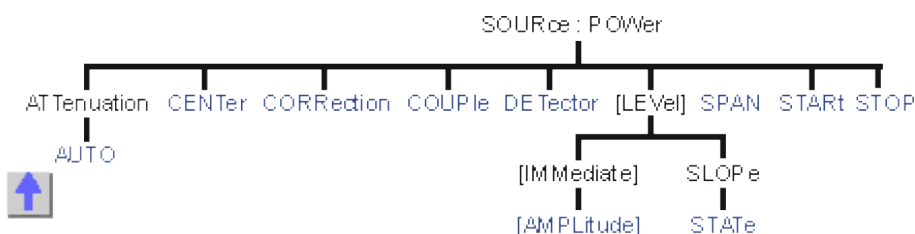

Sometimes the same keyword, such as **STATE**, is used in several branches of the command tree. To keep track of the current branch, the analyzer's command parser uses the following rules:

- **Power On and Reset** - After power is cycled or after \*RST, the current path is set to the root level commands.
- **Message Terminators** - A message terminator, such as a <NL> character, sets the current path to the root command level. Many programming language output statements send message terminators automatically. Message terminators are described in Sending Messages to the Analyzer.
- **Colon (:)** - When a colon is between two command keywords, it moves the current path down one level in the command tree. For example, the colon in :SOURCE:POWER specifies that POWER is one level below SOURCE. When the colon is the first character of a command, it specifies that the following keyword is a root level command. For example, the colon in :SOURCE specifies that source is a root level command.

**Note:** You can omit the leading colon if the command is the first of a new program line. For example, the following two commands are equivalent:

```
SOUR:POW:ATT:AUTO
:SOUR:POW:ATT:AUTO
```

- **<WSP>** - Whitespace characters, such as <tab> and <space>, are generally ignored. There are two important exceptions:
  - Whitespace inside a keyword, such as :CALC ULATE, is not allowed.
  - Most commands end with a parameter. You must use whitespace to separate these ending parameters from commands. **Always refer to the command documentation.** In the following example, there is whitespace between STATE and ON .

```
CALCULATE1:SMOOTHING:STATE ON
```

- **Comma (,)** - If a command requires more than one parameter, you must separate adjacent parameters using a comma. For example, the SYSTEM:TIME command requires three values to set the analyzer clock: one for hours, one for minutes, and one for seconds. A message to set the clock to 8:45 AM would be SYSTEM:TIME 8,45,0. Commas do not affect the current path.
- **Semicolon(;)** - A semicolon separates two commands in the same message without changing the current path. See [Multiple Commands](#) later in this topic.
- **IEEE 488.2 Common Commands** - Common commands, such as \*RST, are not part of any subsystem. An instrument interprets them in the same way, regardless of the current path setting.


## Command and Query

A SCPI command can be an Event command, Query command (a command that asks the analyzer for information), or both. The following are descriptions and examples of each form of command. GPIB Command Finder lists every SCPI command that is recognized by the analyzer, and its form.

| Form                                                                                                                    | Examples                                                                  |
|-------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------|
| <b>Event commands</b> - cause an action to occur inside the analyzer.                                                   | <code>:INITIATE:IMMEDIATE</code>                                          |
| <b>Query commands</b> - query only; there is no associated analyzer state to set.                                       | <code>:SYSTEM:ERROR?</code>                                               |
| <b>Command and query</b> - set or query an analyzer setting. The query form appends a question mark (?) to the set form | <code>:FORMat:DATA ! Command</code><br><code>:FORMat:DATA? ! Query</code> |

## Multiple Commands

You can send multiple commands within a single program message. By separating the commands with semicolons the current path does not change. The following examples show three methods to send two commands:

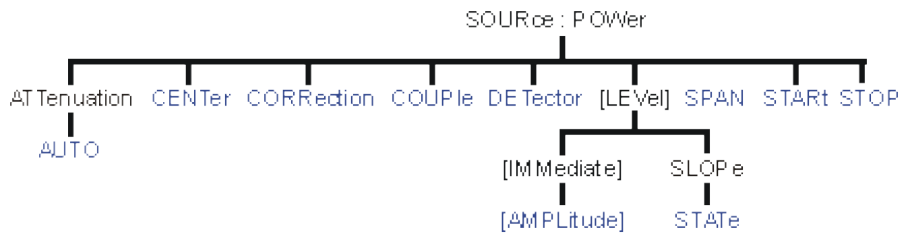

1. **Two program messages:**

```
SOURCE:POWER:START 0DBM
SOURCE:POWER:STOP 10DBM
```

2. **One long message.** A colon follows the semicolon that separates the two commands causing the command parser to reset to the root of the command tree. As a result, the next command is only valid if it includes the entire keyword path from the root of the tree:

```
SOURCE:POWER:START 0DBM;:SOURCE:POWER:STOP 10DBM
```

3. **One short message.** The command parser keeps track of the position in the command tree. Therefore, you can simplify your program messages by including only the keyword at the same level in the command tree.

```
SOURCE:POWER:START 0DBM;STOP 10DBM
```

### Common Commands and SCPI Commands

You can send Common commands and SCPI commands together in the same message. (For more information on these types of commands see [GP-IB Fundamentals](#).) As in sending multiple SCPI commands, you must separate them with a semicolon.

**Example** of Common command and SCPI commands together

```
*RST;SENSE:FREQUENCY:CENTER 5MHZ;SPAN 100KHZ
```

### Command Abbreviation

Each command has a long form and an abbreviated short form. The syntax used in this Help system use uppercase characters to identify the short form of a particular keyword. The remainder of the keyword is lower case to complete the long form.

```
SOUR - Short form
SOURCE - Long form
```

Either the complete short form or complete long form must be used for each keyword. However, the keywords used to make a complete SCPI command can be a combination of short form and long form.

The following is **unacceptable** - The first three keywords use neither short or long form.

```
SOURc:POwe:Atten:Auto on
```

The following is **acceptable** - All keywords are either short form or long form.

```
SOUR:POWer:ATT:Auto on
```

In addition, the analyzer accepts lowercase and uppercase characters as equivalent as shown in the following equivalent commands:

```
source:POW:att:auto ON
Source:Pow:Att:Auto on
```

## Optional [Bracketed] Keywords

You can omit some keywords without changing the effect of the command. These optional, or default, keywords are used in many subsystems and are identified by brackets in syntax diagrams.

### Example of Optional Keywords

The `HCOPY` subsystem contains the optional keyword `IMMEDIATE` at its first branching point. Both of the following commands are equivalent:

```
"HCOPY:IMMEDIATE"
"HCOPY"
```

The syntax in this Help system looks like this:

```
HCOPY[:IMMEDIATE]
```

## Vertical Bars | Pipes

Vertical bars, or "pipes", can be read as "**or**". They are used in syntax diagrams to separate alternative parameter options.

### Example of Vertical Bars:

```
SOURCE:POWER:ATTenuation:AUTO <on|off>
```

Either `ON` or `OFF` is a valid parameter option.

## MIN and MAX Parameters

The special form parameters "`MINimum`" and "`MAXimum`" can be used with **some** commands in the analyzer, as noted in the command documentation. The short form (`min`) and long form (`minimum`) of these two keywords are equivalent.

- **MAX**imum refers to the largest value that the function can currently be set to
- **MIN**imum refers to the smallest value that the function can currently be set to.

**For example**, the following command sets the start frequency to the smallest value that is currently possible:

```
SENS:FREQ:START MIN
```

In addition, the max and min values can also be queried for these commands.

**For example**, the following command returns the smallest value that Start Frequency can currently be set to:

```
SENS:FREQ:START? MIN
```

An error will be returned if a numeric parameter is sent that exceeds the `MAX` and `MIN` values.

**For example**, the following command will return an "Out of range" error message.

```
SENS:FREQ:START 1khz
```



## Getting Data from the Analyzer

---

Data is sent from the analyzer in response to program queries. Data can be short response messages, such as analyzer settings, or large blocks of measurement data. This topic discusses how to read query responses and measurement data from the analyzer in the most efficient manner.

### [Response Message Syntax](#)

### [Clearing the Output Queue](#)

### [Response Data Types](#)

### [Transferring Measurement Data](#)

---

**Note:** Some PCs use a modification of the IEEE floating point formats with the byte order reversed. To reverse the byte order for data transfer into a PC, use the `FORMat:BORe` command.

---

## Other Topics about GPIB Concepts

### Response Message Syntax

Responses sent from the analyzer contain data, appropriate punctuation, and message terminators.

`<NL><^END>` is always sent as a response message terminator. Most programming languages handle these terminators transparent to the programmer.

Response messages use commas and semicolons as separators in the following situations:

- a comma separates response data items when a single query command returns multiple values

```
FORM:DATA? 'Query
ASC, +0 'Analyzer Response
```

- a semicolon separates response data when multiple queries are sent within the same messages



```
SENS:FREQ:STAR?;STOP? --Example Query
+1.23000000E+008; +7.89000000E+008<NL><^END> 'Analyzer Response
```

### Clearing the Output Queue

After receiving a query, the analyzer places the response message in its output queue. Your program should read the response immediately after the query is sent. This ensures that the response is not cleared before it is read. The response is cleared when one of the following conditions occur:

- When the query is not properly terminated with an ASCII carriage return character or the GPIB `<^END>` message.
- When a second program query is sent.
- When a program message is sent that exceeds the length of the input queue
- When a response message generates more response data than fits in the output queue.
- When the analyzer is switched ON.

## Response Data Types

The analyzer sends different response data types depending on the parameter being queried. You need to know the type of data that will be returned so that you can declare the appropriate type of variable to accept the data. For more information on declaring variables see your programming language manual. The GPIB Command Finder lists every GPIB command and the return format of data in response to a query. The analyzer returns the following types of data:

### Numeric Data

### Character Data

### String Data

### Block Data

#### Numeric Data

All numeric data sent over the GPIB is ASCII character data. Your programming environment may convert the character data to numeric data for you. Boolean data (1 | 0) is a type of numeric data.

#### Character Data

Character data consists of ASCII characters grouped together in mnemonics that represent specific analyzer settings. The analyzer always returns the short form of the mnemonic in upper-case alpha characters. Character data looks like string data. Therefore, refer to the GPIB Command Finder to determine the return format for every command that can be queried.

#### Example of Character Data

```
MLOG
```

#### String Data

String data consists of ASCII characters. String parameters can contain virtually any set of ASCII characters. When sending string data to the analyzer, the string **must** begin with a single quote ( ' ) or a double quote ( " ) and end with the same character (called the delimiter).

---

**Note:** The analyzer responds best to all special characters if the string is enclosed in single quotes. If quotes are not used, the analyzer will convert the text to uppercase. The analyzer may not respond as you expect.

---

The analyzer always encloses data in double quotes when it returns string data.


#### Example of String Data

```
GPIB.Write "DISP:WINDow:TITLe:DATA?"
```

```
"This is string response data."
```

#### Block Data

Block data is used to transfer measurement data. Although the analyzer will accept either definite length blocks or indefinite length blocks, it always returns definite length block data in response to queries unless the specified format is ASCII. The following graphic shows the syntax for definite block data:

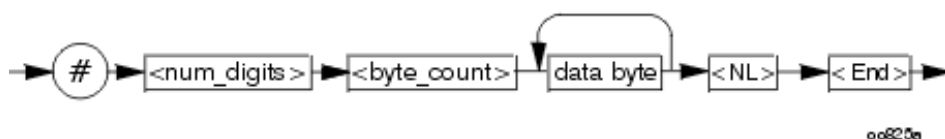

<num\_digits> specifies how many digits are contained in <byte\_count>  
<byte\_count> specifies how many data bytes will follow in <data bytes>

### Example of Definite Block Data

```
#17ABC+XYZ<nl><end>
```

# - always sent before definite block data

1 - specifies that the byte count is one digit (7)

7 - specifies the number of data bytes that will follow, not counting <NL><END>

<NL><END> - always sent at the end of block data


### Transferring Measurement Data

Measurement data is blocks of numbers that result from an analyzer measurement. Measurement data is available from various processing arrays within the analyzer. For more information on the analyzer's data processing flow, see [Accessing Data Map](#). Regardless of which measurement array is read, transferring measurement data is done the same.

When transferring measurement data, the FORMat:DATA command allows you to choose from the following two data types:

- REAL
- ASCII

The following graphic shows the differences in transfer times between the two:

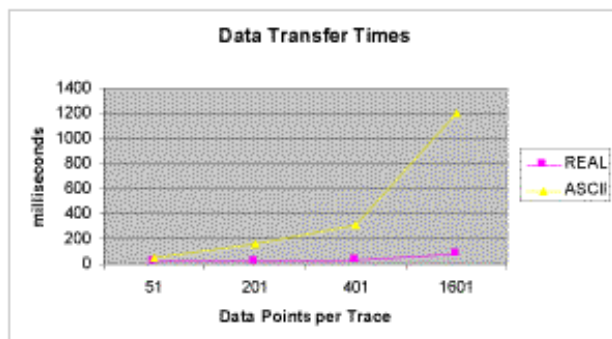

### REAL Data

REAL data (also called floating-point data) types transfer faster. This is because REAL data is binary and takes about half the space of ASCII data. The disadvantage of using REAL data is that it requires a header that must be read. See [definite length block data](#). The binary floating-point formats are defined in the IEEE 754-1985 standard. The following choices are available in REAL format:

- **REAL,32** - IEEE 32-bit format - single precision (not supported by HP BASIC)
- **REAL,64** - IEEE 64-bit format - double precision

### ASCII Data

The easiest and slowest way to transfer measurement data is to use ASCII data. ASCII data is sent if the data contains both numbers and characters (the setting of FORMat:DATA is ignored). ASCII data is separated by commas.

## Understanding Command Synchronization

---

The analyzer takes more time to process some commands than others:

- **Sequential** commands are processed quickly and in the order in which they are received.
- **Overlapped** commands take longer to process. Therefore, they allow the program to do other tasks while waiting. However, the programmer may want to prevent the analyzer from processing new commands until the overlapped command has completed. This is called "synchronizing" the analyzer and controller.

---

**Note:** The analyzer has two overlapped commands:

**INITiate:IMMEDIATE**

**SENSe:SWEep:MODE GROUPS** (when INIT:CONT is ON)

---

The analyzer's queues store commands and responses waiting to be processed. Using the analyzer's queues and controlling the processing sequence of overlapped commands is called synchronizing the analyzer and the controller. This topic discusses how and when synchronizing should be performed.

### Analyzer Queues

### Synchronizing Overlapped Commands

## Other Topics about GPIB Concepts

### Analyzer Queues

Queues are memory buffers that store messages until they can be processed. The analyzer has the following queues:

#### Input Queue

#### Output Queue

#### Error Queue



#### Input Queue

The controller sends statements to the analyzer without regard to the amount of time required to execute the statements. The input queue is very large (31k bytes). It temporarily stores commands and queries from the controller until they are read by the analyzer's command parser. The input queue is cleared when the analyzer is switched ON.

#### Output Queue

When the analyzer parses a query, the response is placed in the output queue until the controller reads it. Your program should immediately read the response or it may be cleared from the output queue. The following conditions will clear a query response:

- When a second query is sent before reading the response to the first. This does not apply when multiple queries are sent in the same statement.
- When a program statement is sent that exceeds the length of the input queue.

- When a response statement generates more data than fits in the output queue.
- When the analyzer is switched ON.

## Error Queue

Each time the analyzer detects an error, it places a message in the error queue. When the `SYSTEM:ERROR?` query is sent, one message is moved from the error queue to the output queue so it can be read by the controller. Error messages are delivered to the output queue in the order they were received. The error queue is cleared when any of the following conditions occur:

- When the analyzer is switched ON.
- When the `*CLS` command is sent to the analyzer.
- When all of the errors are read.

If the error queue overflows, the last error is replaced with a "Queue Overflow" error. The oldest errors remain in the queue and the most recent error is discarded.

## Synchronizing Overlapped Commands

GPIB commands are executed and processed by the analyzer in the order they are received. Commands can be divided into two broad classes:

- **Overlapped commands** generally take extended time to process by the analyzer. Examples of functions that have overlapped commands are printing and making measurements. Because they take longer to process, they allow the execution of subsequent commands while the overlapped command is still in progress. However, the programmer may want to prevent the analyzer from processing new commands until the overlapped command has completed. This is called "synchronizing" the analyzer and controller.
- **Sequential commands** are generally processed quickly by the analyzer. Therefore, they prevent the processing of subsequent commands until the sequential command has been completely processed. **These commands do NOT require synchronization.**

### Synchronization Methods

#### When To Synchronize

### Synchronization Methods

The following common commands are used to synchronize the analyzer and controller. Examples are included that illustrate the use of each command in a program. See the SCPI command details to determine if a command is an overlapped command.

\*WAI

\*OPC?

\*OPC

\*WAI

The \*WAI command:

- **Stops the analyzer** from processing subsequent device commands until all overlapped commands are completed.

- It does **NOT** stop the controller from sending commands to this and other devices on the bus. This is the easiest method of synchronization.


### Example of the \*WAI command

```

GPiB.Write "ABORT;:INITIATE:IMMEDIATE" 'Restart the measurement.
GPiB.Write "CALCULATE:MARKER:SEARCH:MAXIMUM" 'Search for max amplitude.
GPiB.Write "CALCULATE:MARKER:X?" 'Which frequency?

```

The following timeline shows how the processing times of the three commands relate to each other:

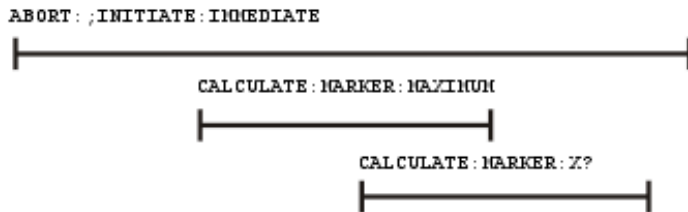

INITIATE:IMMEDIATE is an overlapped command; it allows the immediate processing of the sequential command, CALCULATE:MARKER:SEARCH:MAXIMUM. However, the INITIATE:IMMEDIATE is not considered complete until the measurement is complete. Therefore, the marker searches for maximum amplitude before the measurement completes. **The CALCULATE:MARKER:X? query could return an inaccurate value.**


To solve the problem, insert a \*WAI command.

```

GPiB.Write "ABORT;:INITIATE:IMMEDIATE" 'Restart the measurement.
GPiB.Write "*WAI" 'Wait until complete.
GPiB.Write "CALCULATE:MARKER:SEARCH:MAXIMUM" 'Search for max amplitude.
GPiB.Write "CALCULATE:MARKER:X?" 'Which frequency?

```

The timeline now looks like this:

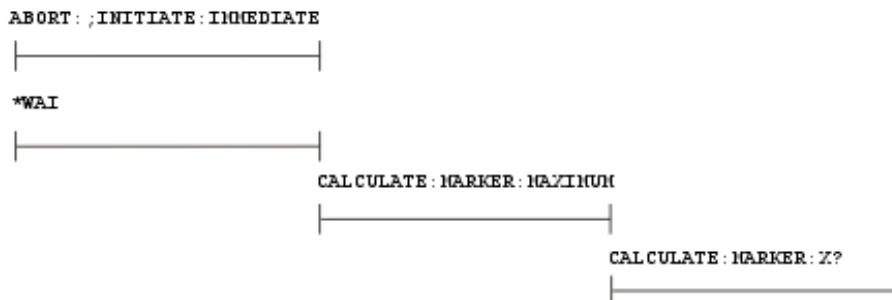

The \*WAI command keeps the MARKER:SEARCH:MAXIMUM from taking place until the measurement is completed. The CALCULATE:MARKER:X? query returns the correct value.

---

**Note:** Although \*WAI stops the analyzer from processing subsequent commands, it does not stop the controller. The controller could send commands to other devices on the bus.

---

### \*OPC?

The \*OPC? query stops the controller until all pending overlapped commands are completed.

In the following example, the **Read** statement following the \*OPC? query will not complete until the analyzer responds, which will not happen until all pending overlapped commands have finished. Therefore, the analyzer and other devices receive no subsequent commands. A "1" is placed in the analyzer output queue when the analyzer completes processing an overlapped command. The "1" in the output queue satisfies the **Read** command and the program continues.

### Example of the \*OPC? query

This program determines which frequency contains the maximum amplitude.

```

GPiB.Write "ABORT; :INITIATE:IMMEDIATE"! Restart the measurement

```

```
GPIB.Write "*OPC?" 'Wait until complete
Meas_done = GPIB.Read 'Read output queue, throw away result
GPIB.Write "CALCULATE:MARKER:MAX" 'Search for max amplitude
GPIB.Write "CALCULATE:MARKER:X?" 'Which frequency?
Marker_x = GPIB.Read
PRINT "MARKER at " & Marker_x & " Hz"
```

## **\*OPC**

The \*OPC command allows the analyzer and the controller to process commands while processing the overlapped command.

When the analyzer completes processing an overlapped command, the \*OPC command sets bit 0 of the standard event register to 1. This requires polling of status bytes or use of the service request (SRQ) capabilities of your controller. See [Reading the Analyzer's Status Registers](#) for more information about the standard event status register, generating SRQs, and handling interrupts.

---

**Note:** Be careful when sending commands to the analyzer between the time you send \*OPC and the time you receive the interrupt. Some commands could jeopardize the integrity of your measurement. It also could affect how the instrument responds to the previously sent \*OPC.

---

**Example of polled bit and SRQ processes.**

## **When To Synchronize the Analyzer and Controller**

Although a command may be defined as an overlapped command, synchronization may not be required. The need to synchronize depends upon the situation in which the overlapped command is executed. The following section describes situations when synchronization is required to ensure a successful operation.

### **Completion of a Measurement**

#### **Measurements with External Trigger**

#### **Averaged Measurements**

### **Completion of a Measurement**

To synchronize the analyzer and controller to the completion of a measurement, use the `ABORT; INITIATE: IMMEDIATE` command sequence to initiate the measurement.

This command sequence forces data collection to start (or restart) under the current measurement configuration. A restart sequence, such as `ABORT; INITIATE: IMMEDIATE` is an overlapped command. It is complete when all operations initiated by that restart command sequence, including the measurement, are finished. The `*WAI`, `*OPC?` and `*OPC` commands allow you to determine when a measurement is complete. This ensures that valid measurement data is available for further processing.

### **Measurements with External Trigger**

To use an external trigger, synchronize the analyzer and controller before the trigger is supplied to the measurement. Setup the analyzer to receive a trigger from an external source (wired to the EXTERNAL TRIGGER connector on the rear panel). The trigger system is armed by GPIB with `INITIATE: IMMEDIATE`. (Because the source of the trigger has been specified as external, this command "readies" the analyzer for a trigger but it does not actually generate the trigger.).

### **Averaged Measurements**

Averaged measurements are complete when the average count is reached. The average count is reached when the specified number of individual measurements is combined into one averaged measurement result. Use synchronization to determine when the average count has been reached.

If the analyzer continues to measure and average the results after the average count is reached, use synchronization to determine when each subsequent measurement is complete.

---



## Reading the Analyzer's Status Register

---

The PNA has several status registers that your program can read to know when specific events occur. There are two methods of reading the status registers in the analyzer: the Polled Bit method and the Service Request method.

### Polled Bit Method

### Service Request Method

### Setting and Reading Bits in Status Registers

### Positive and Negative Transitions


### Status Commands

---

#### Other Topics about GPIB Concepts

---

Most of the status registers in the analyzer have sixteen bits. For simplicity, this topic will illustrate their use with 8-bit registers. Bits in registers represent the status of different conditions inside of the analyzer. In the following graphic, a register is represented by a row of boxes; each box represents a bit. Bit 3 is ON.



---

### The Polled Bit Method

With the Polled Bit Method, your program **continually** monitors a bit in the status register that represents the condition of interest to you. When the analyzer sets the bit to 1, your program immediately sees it and responds accordingly.

**Advantage:** This method requires very little programming.

**Disadvantage:** This method renders your program unavailable to do anything other than poll the bit of interest until the condition occurs.

#### Procedure:

1. Decide which condition to monitor. The Status Commands topic lists all of the possible conditions that can be monitored in the analyzer.
  2. Determine the command and the bit that will monitor the command.
  3. Construct a loop to poll that bit until it is set.
  4. Construct the routine to respond when the bit is set.
- 

### The Service Request (SRQ) Method

Your program enables the bits in the status registers representing the condition of interest. When the condition occurs, the analyzer actively interrupts your program from whatever it is doing, and an event handler in your program responds accordingly. Do this method if you have several conditions you want to monitor or the conditions are such that it is not practical to wait for the condition to occur.

**Advantage:** This method frees your program to do other things until the condition occurs. The program is interrupted to respond to the condition.

**Disadvantage:** This method can require extensive programming depending on the number and type of conditions

that you want to monitor.

### Procedure:

1. Decide which conditions to monitor. The [Status Commands](#) topic lists all of the possible analyzer conditions that can be monitored.
2. Set the enable bits in the **summary** registers and the **status byte** register.

**Enabling** is like making power available to a light - without power available, the switch can be activated, but the light won't turn ON. In the analyzer, without enabling, the condition may occur, but the controller won't see it unless it is enabled.

The condition, and the bit in the **summary** registers in the reporting path, must be enabled. This is like streams (conditions) flowing into rivers (summary registers), and rivers flowing into the ocean (controller). See the diagram of status registers in [Status Commands](#).

Bit 6 of the **status byte** register is the only bit that can interrupt the controller. When **any** representative bit in the status byte register goes ON, bit 6 is automatically switched ON.

3. Enable your program to interrupt the controller. This is done several ways depending on the programming language and GPIB interface card you use. An [example program](#) is provided showing how this is done with in Visual Basic with a National Instruments GPIB card.
4. Construct a subroutine to handle the interrupt event. If you are monitoring more than one condition in your system, your event handler must determine which condition caused the interrupt. Use the \*SPE command to determine the instrument that caused the interrupt, then poll the summary registers, then poll condition registers to determine the cause of the interrupt.

---

### Setting and Reading Bits in Status Registers

Both methods for reading status registers requires that you read bits out of the status registers. Most of the PNA status registers contain 16 bits, numbered 0 to 15. Each bit has a weighted value. The following example shows how to set the bits in a 8-bit status register.

8-bit register

| Bit    | 0 | 1 | 2 | 3 | 4  | 5  | 6  | 7   |
|--------|---|---|---|---|----|----|----|-----|
| Weight | 1 | 2 | 4 | 8 | 16 | 32 | 64 | 128 |

We want to set bits 4 and 5 in the Standard Event Status Enable register.

| Step                                                                                                  | Example                          |
|-------------------------------------------------------------------------------------------------------|----------------------------------|
| 1. Read the weighted bit value for these bits                                                         | weights 16 and 32 (respectively) |
| 2. Add these values together                                                                          | $16 + 32 = 48$                   |
| 3. Send this number as an argument in the appropriate command. (see <a href="#">Status Commands</a> ) | STAT:QUES:LIMIT1:ENAB 48         |

---

### Positive and Negative Transitions

Transition registers control what type of in a condition register will set the corresponding bit in the event register.

- **Positive** transitions (**0 to 1**) are only reported to the event register if the corresponding positive transition bit is set to 1.
- **Negative** transitions (**1 to 0**) are only reported to the event register if the corresponding negative transition bit is set to 1.

- Setting **both** transition bits to 1 causes both **positive and negative** transitions to be reported.

Transition registers are read-write and are unaffected by \*CLS (clear status) or queries. They are reset to their default settings at power-up and after \*RST and SYSTem:PRESet commands. The **following are the default settings** for the transition registers:

- All Positive Transition registers = 1
- All Negative Transition registers = 0

This means that, by default, the analyzer will latch all event registers on the negative to positive transition (0 to 1).

The following is an example of why you would set transition registers:

A critical measurement requires that you average 10 measurements and then restart averaging. You decide to poll the averaging bit. When averaging is complete, the bit makes a positive transition. After restart, you poll the bit to ensure that it is set back from 1 to 0, a negative transition. You set the negative transition bit for the averaging register.

---

## Configure for SCPI LAN using SICL / VISA

---

### [PNA Supported Interfaces](#)

### [Agilent I/O Libraries](#)

### [SICL / VISA Programs Running on the PNA](#)

### [Configure the PNA for SICL / VISA](#)

### [Configure the External Controller](#)

### Other Topics about GPIB Concepts

## PNA Supported Interfaces

The PNA supports the following interfaces for SICL / VISA communication:

- **LAN** - as a remote GPIB interface. The PNA LAN is presented as a virtual GPIB interface. It does NOT support simple TCPIP-based control. Therefore, when configuring the Agilent IO libraries on your PC, add a **REMOTE GPIB** interface, which uses the LAN client interface.
- **GPIB** - requires that your external controller have a GPIB card.

**Note:** For optimum LAN interface performance, use [COM](#) to control the PNA. SCPI commands can be sent to the PNA using the COM [SCPIStringParser](#) object.

The following interfaces are NOT supported:

- **USB** - Although the PNA uses USB to control peripherals, it cannot be controlled over USB.
- **Serial**

### **Important Note:**

To enable VISA or SICL communication over LAN, you must do the following:

1. On the PNA, click **System**, point to **Configure**, then click **SICL/GPIB**.
2. Check **SICL Enabled**. To automatically enable SICL when the PNA is booted, check **Automatically enable on Startup**.
3. Click **OK**.

The PNA is now ready to be controlled over LAN.

[Learn more about this dialog box.](#)

## Agilent I/O Libraries

The Agilent I/O libraries includes the drivers to allow you to communicate with Agilent test instruments. Every PNA

is shipped with the 'M' version of the Agilent I/O libraries installed. We recommend you do NOT upgrade the Agilent I/O libraries on the PNA as unexpected result may occur. If you choose to upgrade the Agilent I/O libraries on the PNA, do NOT change the default folder path in the InstallShield Wizard.

To communicate with the PNA, the Agilent I/O libraries must also be installed on your external controller. To purchase the Agilent I/O libraries, or download a free upgrade, go to [www.agilent.com](http://www.agilent.com) and search for IO Libraries. Scroll to find Software, Firmware & Drivers.

### SICL / VISA Programs Running on the PNA

You can run your SICL / VISA program on the PNA to control the PNA. Although the Agilent I/O libraries are already installed on the PNA, it is configured as the **Host**. You must also configure a SICL or VISA LAN **Client** interface on the PNA, specifying the LAN hostname of that same PNA.

If your program uses the COM interface to VISA, and is compiled on a PC with the Agilent IO Libraries Suite (version 14 or later), and the resulting executable is copied and run on the PNA, it will produce a "type mismatch error". This is because the PNA has the 'M' version of Agilent I/O libraries. The following Visual Basic code is an example of how to avoid this error when communicating with the PNA from within the PNA:

```
Dim rm As IResourceManager
Dim fmio As IFormattedIO488
Set rm = CreateObject("AgilentRM.SRMcls")
Set fmio = CreateObject("VISA.BasicFormattedIO")
Set fmio.IO = rm.Open("GPIB0::22")
fmio.WriteString "*IDN?" & Chr(10)
MsgBox fmio.ReadString()
```

### Controlling the PNA over LAN while controlling other instruments over GPIB

The PNA can NOT be both a controller and talker/listener on the same GPIB bus. Using SICL / VISA, you can use LAN to control the PNA, leaving the PNA free to use the rear-panel GPIB interface to control other GPIB devices.

### Configure the PNA for SICL / VISA

1. On the PNA, click **System** then check **Windows Taskbar**
2. Click **Start** then point to **Program Files, Agilent IO Libraries**, then click **IO Config**
3. Select each GPIB Interface and click **Edit** to verify (or make) the default settings in the following table. These settings are REQUIRED when using a [82357A USB / GPIB](#) Interface with the PNA.
4. When complete, click **OK** to close the edit dialog.
5. Click **OK** to close the IO Config dialog.

| VISA Interface Name | SICL Interface Name | Dialog box title                  | Description                                                                                                                                                                                                                           |
|---------------------|---------------------|-----------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| GPIB0               | gpib0               | GPIB Using NI-488.2               | PNA Rear-panel GPIB connector. This GPIB interface can be used to control the PNA <b>OR</b> for the PNA to control external equipment. IT CAN NOT DO BOTH IN THE SAME PROGRAM. <a href="#">Learn more about pass-through options.</a> |
| GPIB1               | hpib7               | Internal Instrument Configuration | Internal interface for programs running on the PNA to control itself.                                                                                                                                                                 |

### Configure the External Controller

Please refer to the Agilent I/O libraries documentation to learn how to configure your controller to communicate with the PNA. These links can show you how to find the following PNA information:

- [PNA full computer name](#)
- [GPIB Address](#)
- [IP Address](#)

This [example program](#) can help test your VISA configuration.



## Interface Control

---

The Interface Control feature allows you to send remote commands and data to the following PNA rear-panel Interfaces: GPIB, Material Handler I/O, Test Set I/O, and Auxiliary I/O.

### [Overview](#)

### [How to Access Interface Control Settings](#)

### [Interface Control Dialog Box](#)

### [Z5326A H08 Test Set Commands](#)

## Other Connectivity Topics

### Overview


The Interface Control feature allows you to send data to control external equipment such as GPIB instruments, a material handler, test set, or other equipment, without needing to create a remote program. The PNA manages the timing and required interface setup. See [Rear Panel Tour](#).

- A unique set of control data can be sent for each channel. In addition, a unique set of control data can be sent before the channel sweep starts, and after the sweep ends.
- Interface Control settings can be saved and recalled from the [Interface Control dialog box](#), or with [Instrument State Save and Recall](#).
- Interface Control settings can be copied to other channels using [Copy Channels](#).
- Control data can only be WRITTEN to the interfaces, NOT READ from the interfaces.
- Control data is sent in the following order. This order cannot be changed.


1. [GPIB Interface](#)
2. [Material Handler Interface](#)
3. [Test Set Interface](#)
4. [Aux Interface](#)
5. [Dwell Time](#)



## How to access Interface Control settings

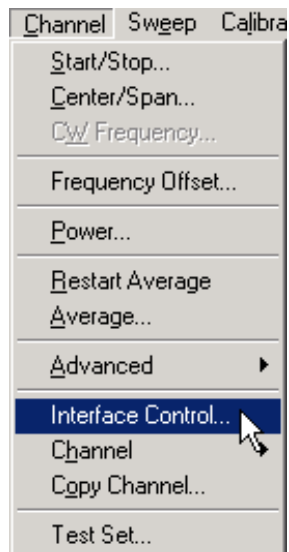

Learn more about using the [front panel interface](#)

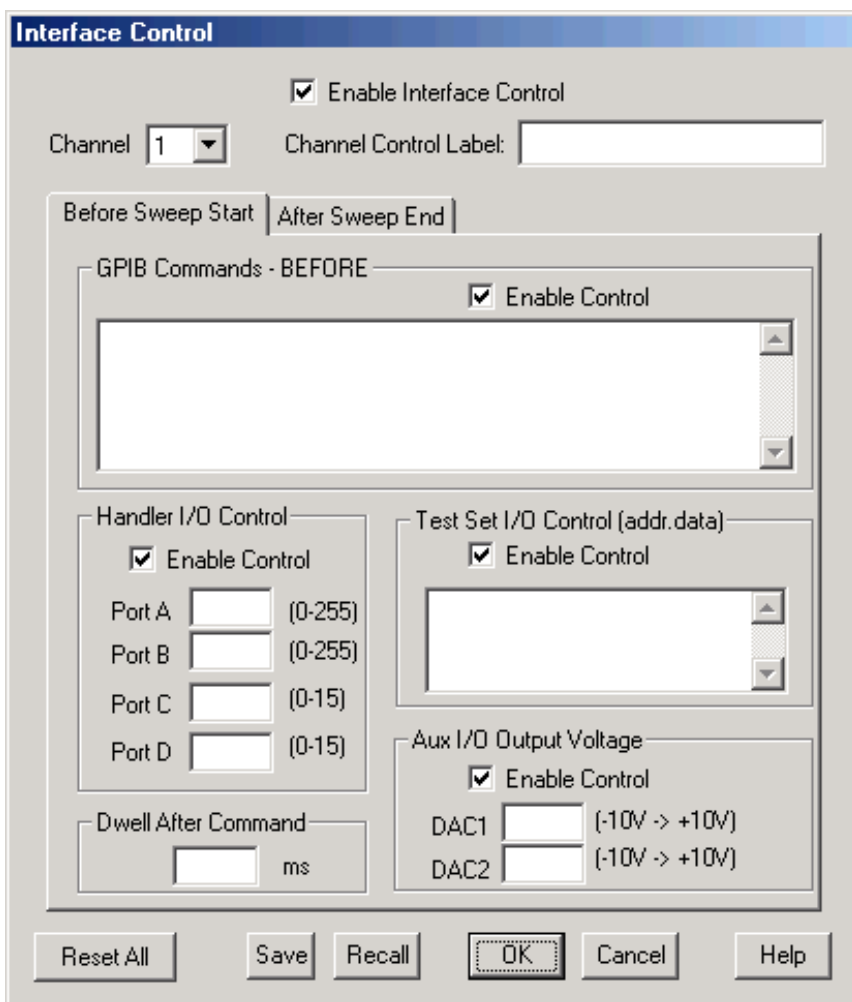

## Interface Control dialog box help

See [Interface Control Overview](#) (scroll up)

An [Instrument Preset](#) will reset all of the fields to their default settings.

**Note:** If an error is encountered when sending Interface Control data, an error message is displayed on the PNA screen. The [Channel Trigger State](#) is set to Hold. You must fix the condition that caused the error, then change the Channel Trigger State to its original setting.

**Enable Interface Control** Enables and disables ALL Interface Control communication. When cleared (default setting) Interface Control is disabled and NO data is sent. To send data, the individual interfaces must also be enabled.

**Channel** Specifies the channel number for dialog settings. Each channel is configured individually. The list box shows the channels that currently have measurements. There must be at least one measurement present in order to make settings.

**Channel Label** Specifies the label to be displayed on the second status bar at the bottom of the PNA screen. The second status bar is automatically displayed when Interface Control is enabled. The remainder of the second status bar is [E5091 Testset status](#).



[Learn about the primary status bar.](#)

### Before Sweep Start - After Sweep End Tabs

Commands / data for all four interfaces can be sent both Before Sweep Start and After Sweep End. However, they are configured and enabled on separate tabs of the Interface Control dialog box. For example, to send GPIB commands both Before and After a PNA sweep, the Enable Control checkbox must be selected and commands entered on BOTH the Before Sweep Start and After Sweep End tabs.

**Before Sweep Start** The data is sent BEFORE the first trace on the channel begins sweeping.

**After Sweep End** The data is sent AFTER the last trace on the channel completes sweeping.

## GPIB Commands

### Notes:

- While using the rear-panel GPIB port with Interface Control, the PNA must be in [GPIB System Controller mode](#). If the PNA is NOT in System Controller mode, an error message appears AND Interface Control is disabled. To correct this situation,
  1. Put the PNA in System Controller mode, and
  2. Re-enable Interface Control.
- GPIB instruments CAN be connected to the PNA using a [USB/GPIB adapter](#). In this case, the PNA can be in talker-listener mode.
- GPIB Queries are NOT supported.

**Enable Control** Enables and disables sending commands out the GPIB interface.

**Multi-line edit control** Each line contains a GPIB command using the following syntax:

```
address command
```

Where:

**address** a number between 0 and 31. The PNA will look through all of the GPIB interfaces for an instrument connected to the specified address. If an instrument with that address is not recognized,

an error is returned.

**command** a GPIB command, with or without enclosing quotes. Enclosing quotes are ignored.

Address and command are separated by at least one space.

Commands should be separated by a new line, or carriage return. For example:

```
19 ":init:cont off"
16 init:imm
```

The front-panel **Enter** key inserts a new line into the field.

The number of GPIB commands that can be entered is limited only by the available memory of the PNA.

See [Z5326A H08 Test Set Commands](#).

## Material Handler I/O

**Enable Control** Enables and disables sending data out the [Material Handler I/O connector](#)

**Ports A, B, C, D** Sends values to the respective Handler I/O port. Although ports C and D are normally bidirectional, ONLY Output mode is allowed using the Interface Control feature. It cannot read from these, or any other, ports.

## Test Set I/O

Note: The PNA has a separate interface for [controlling the E5091A Test Set](#).

**Enable Control** Enables and disables sending data out the [External Test Set I/O connector](#).

**Multi-line edit control** Each line contains a Write command using the following syntax:

```
address.value
```

Where:

**address** any positive integer.

**value** numeric character. Entries that require **alpha** characters should use the [GPIB interface](#).

Address and value are separated by a period. For example:

```
18.2
27.3
```

Entries should be separated by a new line, or carriage return. The PNA front-panel **Enter** key inserts a new line into the field.

All entries are sent out the Test Set I/O port using the [WriteData Method](#).

The number of entries is limited only by the available memory of the PNA.

## Aux I/O

**Enable Control** Enables and disables sending data out the [Auxiliary I/O connector](#).

**DAC1, DAC2** Sets voltages on the Aux I/O connector pins 2 (DAC1) and pin 3 (DAC2).

**Dwell After Command** Specifies a wait time, in milliseconds, after all commands to all interfaces are sent. Any positive integer is allowed. This is used to allow all external devices to settle before beginning a measurement. An erratic trace could indicate that more settling time is necessary.

**Reset All** Sets ALL fields on ALL channels to their default values.

**Save and Recall** Saves and recalls the contents of this dialog box. If the Interface Control dialog box is populated with settings during an [Instrument State Save](#), the settings are automatically recalled with the

Instrument State settings.

Interface control uses an \*.xml file type. An example file is stored on the PNA hard drive. You can recall it into the dialog, or you can open and edit it with a word processor, such as Word Pad.

**OK** Applies the settings and closes the dialog box.

**Cancel** Does not apply changes that were made, and closes the dialog box.

### Z5326A H08 Test Set Commands

The following table lists the commands that are used to control the popular Agilent Z5326A H08 Test Set. These commands can be entered into the [GPIB Interface](#) control.

| Connection Path        | Test Set Command |
|------------------------|------------------|
| Reflection to Port 1   | refl_01          |
| Reflection to Port 2   | refl_02          |
| Reflection to Port 3   | refl_03          |
| Reflection to Port 4   | refl_04          |
| Reflection to Port 5   | refl_05          |
| Reflection to Port 6   | refl_06          |
| Reflection to Port 7   | refl_07          |
| Reflection to Port 8   | refl_08          |
| Transmission to Port 1 | tran_01          |
| Transmission to Port 2 | tran_02          |
| Transmission to Port 3 | tran_03          |
| Transmission to Port 4 | tran_04          |
| Transmission to Port 5 | tran_05          |
| Transmission to Port 6 | tran_06          |
| Transmission to Port 7 | tran_07          |
| Transmission to Port 8 | tran_08          |
| Reset                  | *rst             |
| Reflection Termination | *r_term          |

|                          |           |
|--------------------------|-----------|
| Transmission Termination | *t_term   |
| All Termination          | *all_term |

## Auxiliary I/O Connector

### General Description

This DB-25 male connector provides a variety of analog I/O, digital I/O, timing I/O, and supply lines. You can change the settings on the Auxiliary IO connector through SCPI and COM programming commands. The settings are NOT accessible through the front-panel keys or display menu.

**Note:** The AUX IO configuration settings REMAIN after an Instrument Preset and Hibernation. However, Preset will clear the DAC values. The settings will revert to their default settings ONLY after the PNA is restarted, or until they are changed by you. AUX IO settings are saved and recalled with Instrument State.



| Pin | Name                            | Description                                                       |
|-----|---------------------------------|-------------------------------------------------------------------|
| 1   | <u>ACOM</u>                     | Ground reference for analog signals                               |
| 2   | <u>Analog Out 2</u>             | -10 to +10Vdc output, 10mA max                                    |
| 3   | <u>Analog Out 1</u>             | -10 to +10Vdc output, 10mA max                                    |
| 4   | no connect                      | for future enhancements                                           |
| 5   | <u>DCOM</u>                     | Ground reference for digital signals                              |
| 6   | reserved                        | for future enhancements                                           |
| 7   | reserved                        | for future enhancements                                           |
| 8   | reserved                        | for future enhancements                                           |
| 9   | <u>+5V</u>                      | +5Vdc output, 100mA max.                                          |
| 10  | <u>Pass/Fail Write Strobe</u>   | Indicates pass/fail line is valid (active low)                    |
| 11  | <u>Sweep End</u>                | Indicates sweep is done (programmable modes)                      |
| 12  | <u>Pass/Fail</u>                | Indicates pass/fail (programmable logic, modes and scope)         |
| 13  | <u>Output Port Write Strobe</u> | Writes I/O port data (active low)                                 |
| 14  | <u>Analog In</u>                | -10 to +10VDC analog input                                        |
| 15  | <u>ACOM</u>                     | Ground reference for analog signals                               |
| 16  | <u>Power Button In</u>          | Grounding replicates front panel power button press               |
| 17  | <u>DCOM</u>                     | Ground reference for digital signals                              |
| 18  | <u>Ready for Trigger</u>        | Indicates ready for external trigger (active low)                 |
| 19  | <u>External Trigger In</u>      | Measurement trigger input (programmable to be active high or low) |

|    |                       |                                                      |
|----|-----------------------|------------------------------------------------------|
| 20 | <u>Footswitch In</u>  | Active low input latches a user-readable status bit. |
| 21 | <u>+22V</u>           | +22Vdc output, 100mA max.                            |
| 22 | <u>In/Out port C0</u> | General purpose input / output                       |
| 23 | <u>In/Out port C1</u> | General purpose input / output                       |
| 24 | <u>In/Out port C2</u> | General purpose input / output                       |
| 25 | <u>In/Out port C3</u> | General purpose input / output                       |

---

### ACOM (pins 1, 15)

#### Description

Analog common (ground) - To be used with the Analog Out and Analog In lines.

ACOM and DCOM are connected to system ground at a star ground point inside the analyzer.

---

### Analog Out 1, 2 (pins 2, 3)

#### Description

Two analog outputs programmable to +/-10V;  $I_{out} < 10\text{mA}$ ;  $R_{out} = 100\ \text{ohms}$

12-bit DACs with voltage resolution of approximately 5mV/count.

The DACs are set to constant values using SCPI or COM, and can be read using SCPI or COM commands.

Preset state for both pins is 0 volts.

#### HW Details

Looking into this output pin is a 100-ohm series resistor followed by two diodes tied to +/-15V for static protection, then the output or an op-amp.

The voltage output is provided by a 12-bit DAC with an op amp buffer.

Specifics:

- Maximum output current = 10mA
- Settling time = 3us

#### Timing

The DACs are set after the last data point is measured, during retrace. If the analyzer is in single sweep mode, the DACs are set as part of the presweep process, before the sweep is triggered.

---

### DCOM (pins 5, 17)

#### Description

Digital common (ground).

Used with the digital input and output lines.

ACOM and DCOM are connected to system ground at a star ground point inside the analyzer.

---

### Pins 6, 7, 8

#### Description

Reserved

---

### **+5V (pin 9)**

#### **Description**

+5V nominal output (100mA max).

Protected by self-healing fuse:

---

### **Pass/Fail Write Strobe (pin 10)**

#### **Description**

See [Handler IO connector](#).

---

### **Sweep End (pin 11)**

#### **Description**

See [Handler IO connector](#).

---

### **Pass/Fail (pin 12)**

#### **Description**

See [Handler IO connector](#).

---

### **Output Port Write Strobe (pin 13)**

#### **Description**

See [Handler IO connector](#).

---

### **Analog In (pin 14)**

#### **Description**

Analog input, +/-10V range, Rin=100k ohm

Bandwidth = 40kHz (2-pole lowpass filter).

This analog input may be read using the [SCPI](#) or [COM](#) commands.

#### **HW Details**

Looking into this pin there is 1k-ohm series resistor followed by 100k-ohm resistor to ground, static protection diodes after the 1k resistor limit the signal to +/-15V, then a high impedance buffer and active filter limiting the bandwidth to 40kHz with a lowpass filter.

---

### **Power Button In (pin 16)**

#### **Description**

Short this pin to ground to replicate a front panel power button key press.

#### **HW Details**

Looking into the pin there is a 215-ohm series resistor followed by a 10k pull-up to the 3V standby supply, static protection diodes to the 0V/5V and then connects to the front panel power key circuit.

CAUTION: Because this line is internally pulled up to 3V, it should not be driven by a TTL driver.

#### **Timing**



Grounding this line for 1us to 2 seconds will simulate pressing the front panel power button.

Grounding this line for >4 seconds will perform a hard reset (similar to a personal computer) and is not recommended.

---

### Ready for Trigger (pin 18)

#### Description

TTL output.

Active Low signal indicates that system is ready for an external trigger.

Remains High if system is not in External Trigger mode.

Goes High after an External Trigger is acknowledged.

Goes Low after the system has finished with its measurements, the source has been set up, and the next data point is ready to be measured.

#### HW Details

Looking into this pin there is a 215-ohm series resistor followed by a 10k pullup, diodes to 0V/5V for static protection, then the output of an "ABT" TTL buffer.

This line is enabled only when the analyzer is in External Trigger mode.

Refer to External Trigger In (following pin) for more information.

#### Timing

Refer to [External Trigger In](#) (following pin)

---

### External Trigger In (pin 19)

#### Description

This input accepts level trigger signals (High / Low) on all PNA models, or edge trigger signals on some PNA models.

The external trigger configuration is set from the [front panel](#), [SCPI](#) or [COM](#).

For more information, see [External triggering](#).


A single trigger is achieved by asserting the external trigger for a period from 1us to 50us. Continuous triggering is achieved by holding the external trigger in the "asserted" mode (either Low or High).

#### HW Details

Looking into this pin is a 215-ohm series resistor followed by a 4.64k pullup, 1000pF to ground and then a "FAST" TTL buffer input.

#### Timing

A level trigger width should be between 1us and 50us.

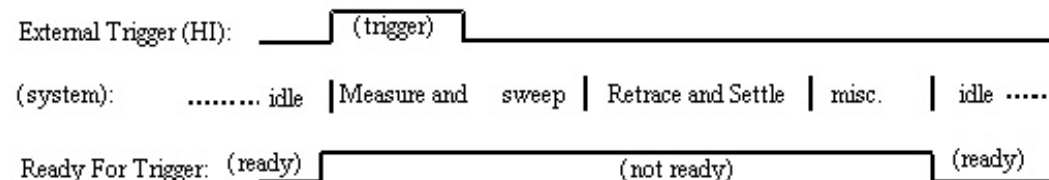

### Footswitch In (pin 20)

#### Description

TTL input.

A Low level input such as shorting this line to ground using a footswitch (where the input stays low for >1us) will be latched.

The latched status may be read using the SCPI or COM commands.

Only one footswitch press can be latched (remembered) by the system.

Reading the latch status will reset it if Footswitch In has returned to a high level.

#### **HW Details**

Looking into this pin is a 215-ohm series resistor followed by a 4.64k pullup to 5V and 1000pF to ground. This line is an input to a "FAST" TTL buffer.

#### **Timing**

Footswitch In must be Low for at least 1us.

---

#### **+22V (pin 21)**

##### **Description**

+22V nominal output (100mA max).  
Protected by self-healing fuse.

---

#### **In/Out Port C0-C3 (pins 22-25)**

##### **Description**

See Handler IO connector

---

## External Test Set I/O Connector

---

### General Description

This DB-25 female connector is used to control external test sets. The external test set bus consists of 13 multiplexed address and data lines, three control lines, and an open-collector interrupt line. The Test Set IO is not compatible with the 8753 test sets.

You can change the settings on the External Test Set IO connector through SCPI and COM programming commands. The settings are NOT accessible through the front-panel keys or display menu.


### Notes:

- The External Test Set pin settings are NOT affected by Instrument State Save/Recall or Instrument Preset.
- At PNA Power Up and return from Hibernation, the External Test Set bus data lines, address lines, and control lines are set HIGH, and no strobe lines are pulsed.

---

**Caution:** Do not mistake this connector with a Parallel Printer port. A printer may be damaged if connected to this port.

---

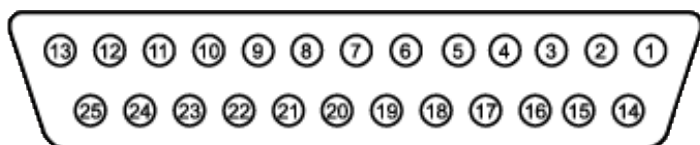

| Pin | Name                    | Description                                            |
|-----|-------------------------|--------------------------------------------------------|
| 1   | <u>SEL0</u>             | Test set select bit 0; tied to GND                     |
| 2   | <u>Sweep Holdoff In</u> | TTL input - state may be read with SCPI or COM command |
| 3   | <u>AD12</u>             | Address and latched data                               |
| 4   | <u>AD10</u>             | Address and latched data                               |
| 5   | <u>AD9</u>              | Address and latched data                               |
| 6   | <u>AD8</u>              | Address and latched data                               |
| 7   | <u>GND</u>              | 0V                                                     |
| 8   | <u>LAS</u>              | TTL output Low = Address Strobe                        |
| 9   | <u>AD4</u>              | Address and latched data                               |
| 10  | <u>AD3</u>              | Address and latched data                               |
| 11  | <u>AD2</u>              | Address and latched data                               |
| 12  | <u>GND</u>              | 0V                                                     |

|    |                     |                                                                                |
|----|---------------------|--------------------------------------------------------------------------------|
| 13 | <u>Interrupt In</u> | TTL input - state may be read with a SCPI or COM command                       |
| 14 | <u>No connect</u>   | <b>CAUTION:</b> Older PNAs have +22v on this line; this will damage a printer. |
| 15 | <u>SEL1</u>         | Test set select bit 1; tied to GND                                             |
| 16 | <u>SEL2</u>         | Test set select bit 2; tied to GND                                             |
| 17 | <u>AD11</u>         | Address and latched data                                                       |
| 18 | <u>SEL3</u>         | Test set select bit 3; tied to GND                                             |
| 19 | <u>AD7</u>          | Address and latched data                                                       |
| 20 | <u>AD6</u>          | Address and latched data                                                       |
| 21 | <u>AD5</u>          | Address and latched data                                                       |
| 22 | <u>AD0</u>          | Address and latched data                                                       |
| 23 | <u>AD1</u>          | Address and latched data                                                       |
| 24 | <u>LDS</u>          | TTL output - active low data strobe                                            |
| 25 | <u>RLW</u>          | TTL output - high-read, low write                                              |

### SEL0-SEL3 (pins 1,15,16,18)

#### Description

Selects addresses of test sets that are "daisy chained" to this port. The select code is set to zero at the PNA connector and is incremented by one as it goes through each successive external test set. Therefore, the first test set in the chain has address zero and so on, for up to 16 test sets.

#### HW Details

Connected to ground inside the PNA.

#### Timing

None

### Sweep Holdoff In (pin 2)

#### Description

Input line used by the test set for holding off a sweep. Holding off a sweep is one way of introducing a delay that allows an external device to settle before the PNA starts taking data. You must write a program that will query the line and perform the delay. The program needs to query the line and keep PNA from sweeping while the line remains low. When a subsequent query detects that the line went high the program would then trigger the PNA to start the sweep.

Use either Single or External trigger mode to control the PNA sweep.

#### HW Details

This pin has a series 215-ohms resistor followed by 4.7k-ohm pull-up and then an "ABT" TTL buffered register.

#### Timing

This input is not latched by the PNA hardware. Therefore the input level must be held at the desired state by the

test set until it's read by your program.

---

### AD0-AD12 (pins 3-6, 9-11, 17, 19-23)

#### Description

Thirteen lines are used to output data addresses or input / output data. Several SCPI and COM commands are available for reading and writing to these lines. You can choose to use commands where the PNA provides the appropriate timing signals needed for strobing the addresses and data. Or you can choose to control the timing signal directly. The timing signals are RLW, LAS and LDS. If you decide to do direct control refer to the corresponding SCPI and COM command details. Close attention to detail is needed to insure the desired results.

After a write command, lines AD0-AD12 are left in the state they were programmed. Default setting for Mode is Read / Input).

After a read command, lines AD0-AD12 are left in input mode. While in this mode an external test set attached to the IO is free to set the level on each line.


#### HW Details

Each of these I/O pins has a series 215-ohm resistor followed by 4.7k-ohm pull-up resistor.


Write/Read is implemented by an output tri-state TTL buffer / latch for latching and enabling write data in parallel with a TTL input buffer for reading.

#### Timing

Output Address and data setup and hold times are 1us minimum.

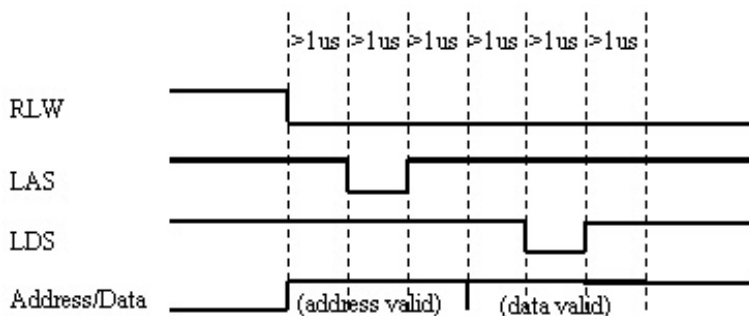

#### Address & Data I/O Write

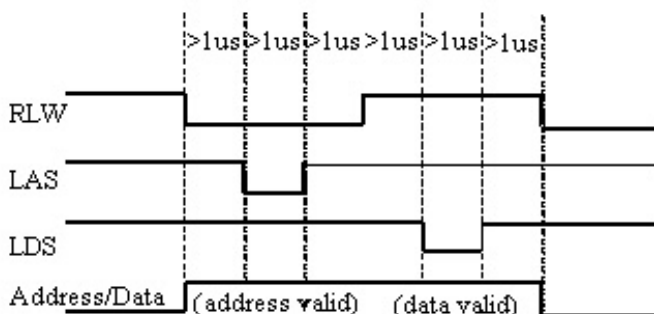

**Address & Data I/O Read** - Data must be valid for 1us before and after strobe

---

### GND (pins 7, 12)

#### Description

Two ground pins used as ground references by the test set.

#### HW Details

Connected to digital ground.

#### Timing

None.

---

### LAS (Low Address Strobe) (pin 8)

#### Description

This line has two behaviors that are command dependent. Refer to the [SCPI](#) and [COM](#) commands for further details.

In one behavior LAS is one of the lines used by the PNA to provide appropriate timing for writing Address and Data to the Test Set. In this case LAS is controlled automatically by the PNA and is intended to be used as the strobe for the Address. When LAS is low, lines AD0 - AD12 represent the Address. LAS will return to its normally high state when the transaction is finished.

In the second behavior the PNA will NOT provide appropriate timing. In this case LAS is controlled directly by the user through a [SCPI](#) or [COM](#) command. When the transaction is finished LAS is left set to the state it was programmed to until another command changes it. (Default for LAS is TTL High).

#### HW Details

This output pin is driven by a TTL latched buffer with a series 215-ohm resistor followed by 2.15k-ohm pull-up.

#### Timing

Strobe length, setup and hold times are all 1us minimum.

See the description for [AD0-AD12](#) for more timing information.

---

### Interrupt In (pin 13)

#### Description

Query this line with a [SCPI](#) or [COM](#) command.

#### HW Details

This line is a non-latched TTL input, has series 215-ohms followed by 4.64k-ohm pullup.

#### Timing

The Test Set must maintain at the desired TTL level until its read.

---

### (pin 14) No Connect (previously +22V )

---

**WARNING:** Early versions of the PNA had +22v on this pin. **Connecting a printer to this port will usually damage the printer.**

---

#### Description

+22V, 100mA max. The 25-pin D connector is the same as a computer parallel printer port connector. Pin (14) corresponds to a printer's "autofeed" line. **Connecting a printer to this port will damage the printer if +22v is present** since printers requires less than 5V on all control lines.

#### HW Details

No connect

#### Timing

None

---

### **LDS (Low Data Strobe) (pin 24)**

#### **Description**

This line has two behaviors that are command dependent. Refer to the External Test Set IO SCPI and COM commands for further details. (Default setting for LDS is TTL High)

In one behavior LDS is one of lines used by the PNA to provide appropriate timing for writing Address and Data to the Test Set. In this case LDS is controlled automatically by the PNA and is intended to be used as the strobe for the Data. When LDS is low, lines AD0 - AD12 represents Data. LDS will return to its normally high state when the transaction is finished.

In the second behavior the PNA will NOT provide appropriate timing. In this case LDS is controlled directly by the user through a SCPI or COM command. When the transaction is finished the LDS is left set to the state it was programmed to.

#### **HW Details**

This output pin is driven by a TTL latched buffer with a series 215-ohm resistor followed by 2.15k-ohm pull-up.

#### **Timing**

Strobe length, setup and hold times are all 1us minimum.

See the description for [AD0-AD12](#) for more timing information.

---

### **RLW (pin 25)**

#### **Description**

This line is the output for the Read Write signal. It has two behaviors that are command dependent. Refer to the External Test Set IO SCPI and COM commands for further details. (Default setting for RLW is TTL High)

In one behavior RLW is controlled automatically by the PNA during a Read Write operation. When RLW is low, lines AD0 - AD12 represent output Data. When RLW is high, the lines represent input Data.

In the second behavior the PNA does NOT provide the timing. The user must control it directly through the SCPI or COM command. In this case the line is left set to the state it was programmed to.

#### **HW Details**

This pin is a TTL latched output with a series 215-ohm resistor followed by 2.15k-ohm pull-up resistor.

#### **Timing**

Strobe length, setup and hold times are all 1us minimum.

See the description for [AD0-AD12](#) for more timing information.

---

## Material Handler I/O Connector

---

This rectangular 36-pin female connector provides communication signals between the PNA and a material parts handler. You can change the settings on the Material Handler IO connector using SCPI and COM commands. The settings are NOT accessible through the front-panel keys or display menu.

### Overview - Controlling a Material Handler

#### Pin Assignments

#### Pin Descriptions

#### Timing Diagrams

#### Input Output Electrical Characteristics

---


**Note:** On early PNAs this connector is labeled "GPIO". It is covered to indicate that the connector is not functional.

---

### Overview - Controlling a Material Handler

The PNA is capable of interacting with an external material handler or part handler. This allows the PNA to be used in an automated test environment, where devices to be tested are inserted into a test fixture by a part handler, and sorted into pass/fail bins by the handler after testing is complete. By connecting the part handler to the PNAs Auxiliary or Material Handler I/O ports, the PNA and part handler can synchronize their activities in a way that makes automated testing possible.

#### PNA and Part Handler Preparation

1. Define the measurements you want to make.
2. Define limits for each of the measurements.
3. Configure the PNAs Material Handler port so that it is compatible with your part handler. This usually involves setting the handler logic, pass/fail logic, pass/fail scope, and pass/fail mode. These settings are made remotely using SCPI or COM commands.
-  4. Use a cable to connect the PNA to your part handler.
5. Put the PNA in External Trigger mode.
6. Load parts in handler per manufacturer instructions.

---


**Note:** The Material Handler configuration settings REMAIN after an Instrument Preset and Hibernation. The settings will revert to their default settings ONLY after the PNA is restarted, or until they are changed by you. Material Handler settings are saved and recalled with Instrument State.

---

#### Flow Diagram

The following diagram and descriptions summarizes the events that occur during automated testing. 'DUT' refers to Device Under Test.



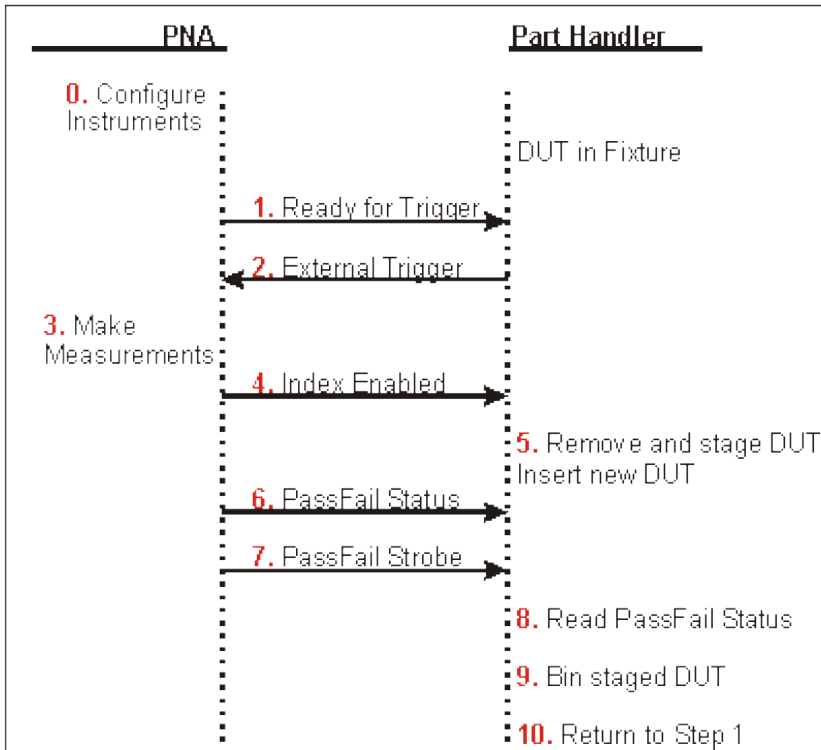

### Text Descriptions

0. (Optional). The PNA sends values out the Material Handler and/or Auxiliary I/O connectors to configure external instruments. The A,B,C, and D ports of the Material Handler can be used to control devices used in testing, such as step attenuators, part handlers, or even the DUT itself. Also, the DAC1 and DAC2 lines on the Aux I/O connector can be used to provide bias voltages for devices and instruments. If you wish to use the Material Handler or Aux connectors for testing, you will need to write a program to send values out the various lines and ports, as there is no activity on these lines by default.
1. The part handler receives a Ready for Trigger signal from the PNA. This indicates that the PNA is properly configured and ready to take a measurement.
2. The part handler sends an External Trigger signal to the PNA. This signals that the part handler has settled, and allows the PNA to begin taking measurements.
3. The PNA takes measurements on all triggerable channels.
4. The Index line on the material handler goes to a Low state, which means that all required data has been collected by the PNA.
5. The part handler removes the DUT from the test fixture, and inserts a new DUT into the fixture. This operation is often referred to as part handler indexing. The device just tested is staged (removed from the fixture and prepared for binning), and the next part to be tested is put into the fixture. The removed DUT cannot be assigned to a Pass/Fail bin yet, as the Pass/Fail status is not available.
6. The PNA sends the Pass/Fail Status.
7. The PNA sends the Pass/Fail Strobe meaning that the Pass/Fail status has been determined.
8. The part handler reads the Pass/Fail Status line.
9. The part handler bins the staged part based on the Pass/Fail Status.
10. The test process repeats at step 1, waiting for Ready for Trigger from the PNA.

## Material Handler IO Pin Assignments



There are three different Handler IO pin assignment configurations depending on the PNA model:

- **Type 1** - All 3 GHz, 6 GHz, and 9 GHz PNA models. You can change the pinout configuration to Type 2 on these models. This requires opening the instrument and changing a connector internally. Refer to the procedure in the Service Guide, Chapter 7. You can download the Service Guide for your PNA model from our website: <http://www.agilent.com>. **Caution:** Changing this connection should be done by qualified service personnel.
- **Type 2** - All PNA models EXCEPT 3 GHz, 6 GHz, and 9 GHz and N5230 Opt 240, 245.
- **Type 3** - N5230 Options: 020,025,120,125, 240, 245

See PNA models and options.

**Shaded/bold** indicates changes from Type 1

**Note:** A slash (/) preceding the signal names indicates that the signal uses negative (active low) logic. A low pulse is a logical 1.

| Pin | Type 1           | Type 2           | Type 3           |
|-----|------------------|------------------|------------------|
| 1   | Ground           | Ground           | Ground           |
| 2   | / INPUT1         | / INPUT1         | / INPUT1         |
| 3   | / OUTPUT1        | / OUTPUT1        | / OUTPUT1        |
| 4   | / OUTPUT2        | / OUTPUT2        | / OUTPUT2        |
| 5   | / Output port A0 | / Output port A0 | / Output port A0 |
| 6   | / Output port A1 | / Output port A1 | / Output port A1 |
| 7   | / Output port A2 | / Output port A2 | / Output port A2 |
| 8   | / Output port A3 | / Output port A3 | / Output port A3 |
| 9   | / Output port A4 | / Output port A4 | / Output port A4 |
| 10  | / Output port A5 | / Output port A5 | / Output port A5 |
| 11  | / Output port A6 | / Output port A6 | / Output port A6 |
| 12  | / Output port A7 | / Output port A7 | / Output port A7 |
| 13  | / Output port B0 | / Output port B0 | / Output port B0 |
| 14  | / Output port B1 | / Output port B1 | / Output port B1 |
| 15  | / Output port B2 | / Output port B2 | / Output port B2 |

|    |                            |                                   |                                                 |
|----|----------------------------|-----------------------------------|-------------------------------------------------|
| 16 | / Output port B3           | / Output port B3                  | / Output port B3                                |
| 17 | / Output port B4           | / Output port B4                  | / Output port B4                                |
| 18 | no connect                 | <b>/ Output port B5</b>           | <b>/ Ext. Trigger</b>                           |
| 19 | / Output port B5           | <b>/ Output port B6</b>           | / Output port B5                                |
| 20 | / Output port B6           | <b>/ Output port B7</b>           | <b>/ Output port B6 -<br/>/ Index Signal</b>    |
| 21 | / Output port B7           | <b>/ In/Out port C0</b>           | <b>/ Output port B7<br/>/ Ready for Trigger</b> |
| 22 | / In/Out port C0           | <b>/ In/Out port C1</b>           | / In/Out port C0                                |
| 23 | / In/Out port C1           | <b>/ In/Out port C2</b>           | / In/Out port C1                                |
| 24 | / In/Out port C2           | <b>/ In/Out port C3</b>           | / In/Out port C2                                |
| 25 | / In/Out port C3           | <b>/ In/Out port D0</b>           | / In/Out port C3                                |
| 26 | / In/Out port D0           | <b>/ In/Out port D1</b>           | / In/Out port D0                                |
| 27 | / In/Out port D1           | <b>/ In/Out port D2</b>           | / In/Out port D1                                |
| 28 | / In/Out port D2           | <b>/ In/Out port D3</b>           | / In/Out port D2                                |
| 29 | / In/Out port D3           | <b>Port C Status</b>              | / In/Out port D3                                |
| 30 | Port C Status              | <b>Port D Status</b>              | Port C Status                                   |
| 31 | Port D Status              | <b>/ Output Port Write Strobe</b> | Port D Status                                   |
| 32 | / Output Port Write Strobe | <b>no connect</b>                 | / Output Port Write Strobe                      |
| 33 | / Pass/Fail                | / Pass/Fail                       | / Pass/Fail                                     |
| 34 | / Sweep End                | <b>+5V</b>                        | / Sweep End                                     |
| 35 | +5V                        | <b>/ Sweep End</b>                | +5V                                             |
| 36 | / Pass/Fail Write Strobe   | / Pass/Fail Write Strobe          | / Pass/Fail Write Strobe                        |

## Pin Descriptions

## Input1

When this Input line receives a Low pulse from the material handler, data is latched on the OUTPUT1 and OUTPUT2 lines. See OUTPUT1|2 Data Output Write Timing

**Note: Type 1 and Type 2 Behavior:** The Input line responds to a High (rising edge) pulse.

The Input Line activity can be read:

| SCPI                          | COM                      |
|-------------------------------|--------------------------|
| <u>CONTrol:HANDler:INPut?</u> | <u>get_Input1 Method</u> |

## Output1, Output2

See OUTPUT1|2 Data Output Write Timing

The **current** state of these latched TTL outputs may be set High or Low (Default setting) using the (non-user) SCPI put\_Output (COM) commands.

The **next** state (following a negative edge on the INPUT1 line) may be pre-loaded to High or Low (Default setting) using the user commands.

For example, on the next negative pulse on the INPUT1 line, you want the OUTPUT1 line to go from 0 to 1. To do this:

```
CONT:HAND:OUTP1:DATA 0 'Force the OUTPUT1 line to 0
CONT:HAND:OUTP1:USER 1 'Set the OUTPUT1:USER buffer to 1, indicating the next
state
```

|                         | SCPI                                  | COM                       |
|-------------------------|---------------------------------------|---------------------------|
| Write User Data         | <u>CONT:HAND:OUTP&lt;pin&gt;:USER</u> | <u>put_Output Method</u>  |
| Read last value written | <u>CONT:HAND:OUTP&lt;pin&gt;:USER</u> | <u>get_Output Method.</u> |
| Write non-user data     | <u>CONT:HAND:OUTP&lt;pin&gt;:DATA</u> | <u>put_Output Method</u>  |
| Read last value written | <u>CONT:HAND:OUTP&lt;pin&gt;:DATA</u> | <u>get_Output Method</u>  |

### Output Ports A and B

These two general purpose, 8-bit output ports are used to write data to the material handler. When any line changes state, all output lines are latched to the I/O connector as the Output Write Strobe goes Low.

The default state for data is Low.

See Data Output Write Timing Diagram

#### Set Port Logic:

The logic for the data lines can be set to either: Positive (1 = High) or Negative (1 = Low). This setting affects all data ports. They cannot be set independently.

**SCPI**

CONTRol:HANDler:LOGic

**COM**

PortLogic Property

#### Combine to read or write data to Port F:

Ports A and B can be virtually combined to write data to one 16-bit I/O port F.

**SCPI**

CONTRol:HANDler:F <num>

**COM**

put Port (F)

### Input/Output Ports C and D

These two general purpose 4-bit Input/Output ports are used to write data (Output) or read data (Input). These lines could be used to write to an external device such as a step attenuator.

When any line changes state, all output lines are latched to the I/O connector as the Output Write Strobe goes Low. See Data Output Write Timing

The four lines of Port C are connected internally to the Auxiliary IO connector.

#### Set Input | Output Mode:

Each port may be independently defined as Output or Input.

**SCPI**

CONTRol:HANDler:C:MODE

CONTRol:HANDler:D:MODE

**COM**

PortMode Property

#### Set Port Logic:

The logic for the data lines can be set to either: Positive (1 = High) or Negative (1 = Low). This setting affects all data ports. They cannot be set independently.

**SCPI**

**COM**

**Read or write data:**

Ports C and D can be virtually combined to read or write data to one 8-bit I/O port **E**. When combined, **both C** and D ports must be set to either INPUT or OUTPUT mode.

**SCPI**

CONTRol:HANDler:<port>[:DATA]>

**COM**

get Port(x)

put Port (x)

**Port C Status, Port D Status**

These two output lines indicate the Read / Write mode of the C and D ports.

- A Low level indicates that the associated port is in **INPUT** mode (read only).
- A High level indicates that the associated port is in **OUTPUT** mode (write only).

These logic of these status outputs cannot be changed.

See Input/Output Ports C and D to learn how to set I/O Mode

See Data Output Write Timing

**Output Port Write Strobe**

This Output line goes Low to write data from Ports A and B and Ports C and D when a change is detected on any of the data lines.

These logic of this strobe output cannot be changed.

This line is shared with Auxiliary IO connector.

See Data Output Write Timing

**External Trigger**

When trigger source is set to external, this Input line accepts a trigger signal from the material handler. This usually means that a part is in place and ready to be tested.

See Trigger Timing Diagram

## Index

A Low signal on this Output line indicates to the material handler that the measurement is complete. This usually means that the handler can connect the next device. However, measurement data is not available until data is calculated. [See Trigger Timing Diagram](#).

### Set Function:

This line also serves as a data line. Set the function using the following commands:

| SCPI                               | COM               |
|------------------------------------|-------------------|
| <u>CONTRol:HANDler:INDex:STATE</u> | <u>IndexState</u> |

## Ready for Trigger

When this output line goes low, it indicates to the material handler that the PNA is ready for a trigger signal.

[See Trigger Timing Diagram](#)

[See Pass/Fail Timing Diagram](#)

### Set Function:

This line also serves as a data line. Set the function using the following commands:

| SCPI                                  | COM                         |
|---------------------------------------|-----------------------------|
| <u>CONTRol:HANDler:RTRigger:STATE</u> | <u>ReadyForTriggerState</u> |

## Pass/Fail State

This Output line indicates to the handler whether the limit test has passed or failed.

Pass/Fail state is valid only when the [limit test](#) function is ON and while [Pass/Fail strobe](#) line is Low. [See Pass/Fail Timing Diagram](#)

This line is shared with the Auxiliary IO connector.

### Set Pass / Fail Logic:

- Positive Logic: High=Pass, Low=Fail. (Default setting)
- Negative Logic: High=Fail, Low=Pass.

| SCPI                                  | COM                           |
|---------------------------------------|-------------------------------|
| <u>CONTRol:HANDler:PASSfail:LOGic</u> | <u>PassFailLogic Property</u> |

### Set Default Conditions:

- **PASS**- the line stays in PASS state. When a device fails, then the line goes to fail after the Sweep End line is asserted.
- **FAIL**- the line stays in FAIL state. When a device passes, then the line goes to PASS state after the Sweep End line is asserted.
- **No Wait**- the line stays in PASS state. When a device fails, then the line goes to fail IMMEDIATELY. (Default setting)

#### SCPI

CONTrol:HANDler:PASSfail:MODE

#### COM

PassFailMode Property

### Set Pass / Fail Scope:

- **Channel scope**: The line resets to the default state after the measurements on a channel have completed.
- **Global scope**: The line resets to the default state after the measurements on all triggerable channels have completed. (Default setting)

#### SCPI

CONTrol:HANDler:PASSfail:SCOPE

#### COM

PassFailScope Property

### Pass/Fail Write Strobe

A Low pulse indicates that Pass/Fail line is valid and the Pass / Fail State is output to the material handler.

This line is shared with the Auxiliary IO connector.

The Pass/Fail Strobe is fixed in duration and timing. However, when the strobe occurs depends on the Pass/Fail Mode and Pass/Fail Scope (Channel or Global) settings. See Pass/Fail State

See Pass/Fail Timing Diagram

### +5V

+5V nominal output (100mA max).

Protected by self-healing fuse.



## Sweep End

This output line indicates the status of the PNA sweep. The sweep includes sweeping the source and taking data.

- **Low** (falling edge) indicates that the specified sweep event has finished. This does NOT indicate that all calculations have finished.
- **High** indicates that the specified sweep event is active.

### See Trigger Timing Diagram

This line is shared with the Auxiliary IO connector.

### Set Sweep Event Mode:

- **Sweep**: indicates that a single source sweep has finished. (Default setting)
- **Channel**: indicates that a single channel has finished.
- **Global**: indicates that all enabled channels have finished.

**SCPI**


CONTRol:HANDler:SWEepend

**COM**

SweepEndMode Property

## Timing Diagrams

### Trigger Timing

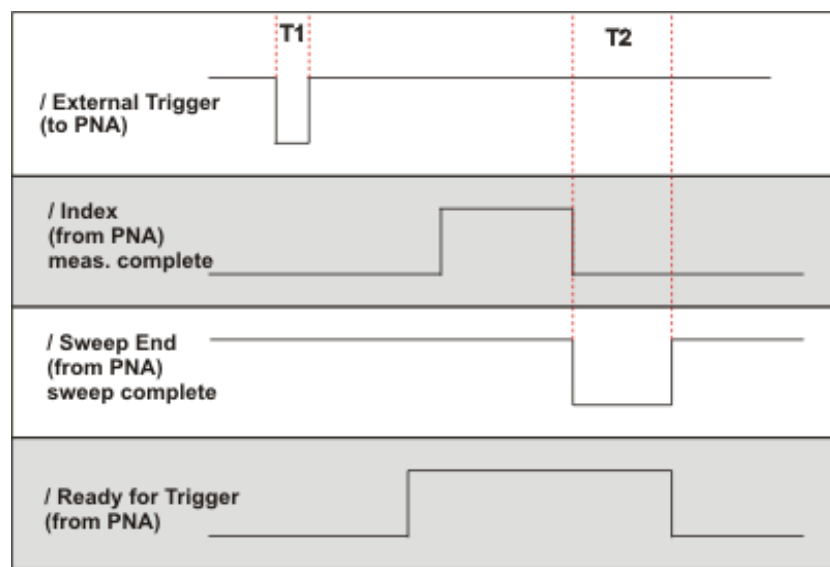


All signals are active low.

**T1 = 1 ms** External Trigger pulse width

**T2 > 10ms** Sweep End pulse width (both High and Low)


### Pass / Fail Timing

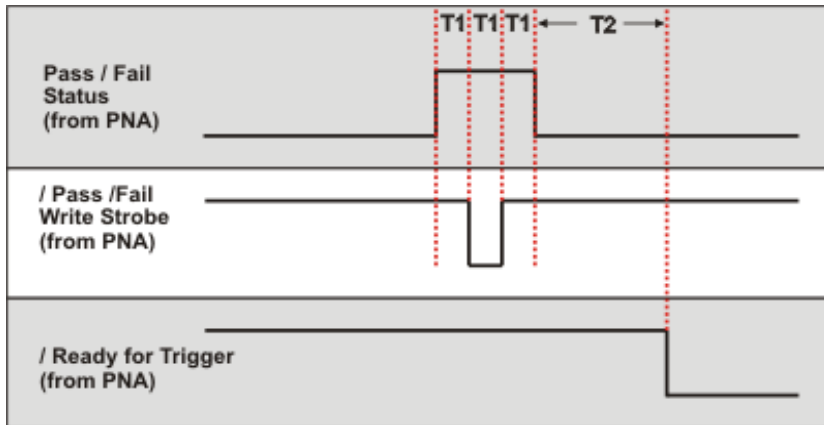

**T1 = 1 ms** Pulse width and response time of Pass / Fail Strobe

**T2 > 10 ms** Ready for Trigger lag


### Ports A-F Data Output Write Timing

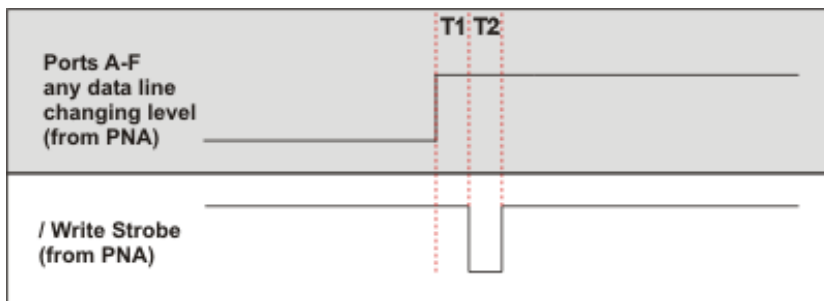

**T1 = 1 ms** Write Strobe response time

**T2 = 1 ms** Write Strobe pulse width

## OUTPUT1|2 Data Output Write Timing

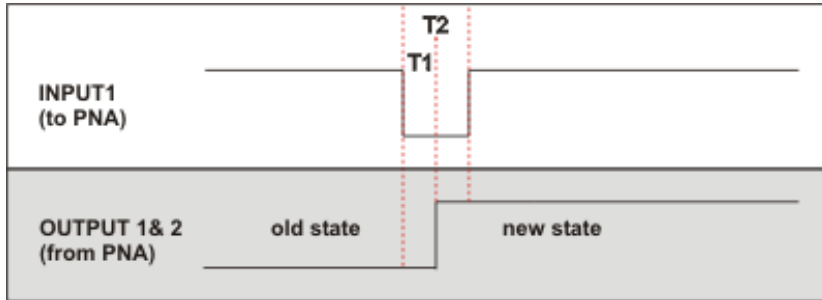

The old state to new state transition can be either low to high (as shown) or high to low.

**T1 = .6 ms** Output1|2 response time

**T2 = 1 ms** Input1 Strobe pulse width

## Input / Output Electrical Characteristics


All Material Handler I/O Input and Output lines are TTL compatible.

### Input and Input/Output lines

Lines carrying information IN (or bidirectional) to the PNA from the material handler.

|                         |                 |
|-------------------------|-----------------|
| Maximum Input Voltages: | -0.5 V to 5.5 V |
| TTL High level:         | 2.0 V to 5.0 V  |
| TTL Low level:          | 0 V to 0.5 V    |

### PNA Input and Input/Output Circuit Diagram

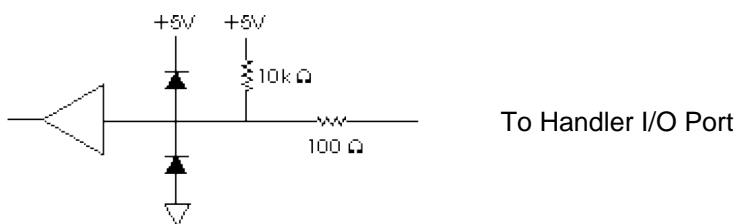


**Note:** The INPUT1 line does NOT have the 10K pullup resistor.

### Output Lines

Lines carrying information OUT of the PNA to the material handler.

|                         |                 |                 |
|-------------------------|-----------------|-----------------|
| Maximum Output Current: |                 | -10 mA to 10 mA |
| Output Current          | TTL High level: | -5 mA           |
|                         | TTL Low level:  | 3 mA            |
| Output Voltage          | TTL High level: | 2.0 V to 3.3 V  |
|                         | TTL Low level:  | 0 V to 0.8 V    |

**PNA Output Circuit Diagram**

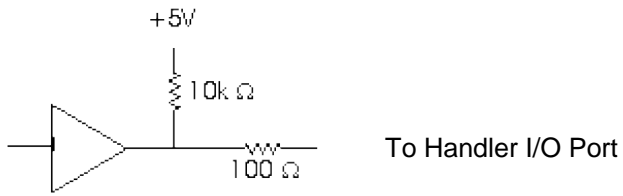

## COM versus SCPI

---

There are two methods you can use to remotely control the PNA: COM and SCPI. The following topics can help you choose the method that best meets your needs:

[Software Connection](#)

[Physical Connection](#)

[Selecting a Method](#)

[Programming Languages](#)

### Other Topics about COM Concepts

#### Software Connection

**COM** uses a binary protocol, allowing you to directly invoke a PNA feature. This is more efficient than SCPI. For example, the following statement calls directly into the PNA, executing the routine `GetIDString`.

```
PNA.GetIDString()
```

**SCPI** is a text based instrument language. To retrieve the ID string, you would send the following text string to the PNA:

```
!bWrite("*IDN?")
```

The PNA SCPI parser would first decode this text string to determine that the user has asked for the PNA to identify itself. Then the parser would call `GetIDString()`.

#### The Physical Connection

##### Internal Control

With either COM or SCPI, the best throughput is attained by using the PNA's internal PC to execute your test code. However, if your test code uses too much system resources (CPU cycles and/or memory), this will slow the PNA's performance.

 Using the SIDL I/O Libraries, you can also connect to the PNA from a program running on the PNA.

##### External Control

You can control the PNA from a remote PC using either COM or SCPI.

**COM** - (Component Object Model) can be used to access any program like the PNA (835x.exe) or library (.dll) that exposes its features using a COM compliant object model. These programs or libraries are called "servers". Programs (like your remote program on your PC) that connect to and use the features of these servers are called "clients."

With COM, the server and the client do not need to reside on the same machine. DCOM, or distributed COM, is easy to configure and makes the location of the server transparent to the client. When you access the PNA from a remote computer, you are using DCOM. In this case, the mechanical transport is a LAN (local area network).

**SCPI** - Using a GPIB interface card in a remote computer, you can connect to the instrument using a GPIB cable. There are some constraints on the length of this cable and the number of instruments that can be daisy-chained together.

Using the Agilent SIDL I/O libraries, you can connect to the instrument over a LAN connection.

(LAN or INTERNAL) You can send SCPI commands using COM with the [ScpiStringParser](#) object.

## Selecting a Method

You should almost always choose COM for the following reasons:

- COM executes faster most of the time.
- COM is generally easier to use. The latest development tools embrace COM and know how to make your life easier with integrated development environments that show automation syntax as you type.
- As time goes on, more emphasis will be put on COM as the preferred programming paradigm.

But choosing a connection method depends on your situation. Here are some additional things to consider:

1. If you want to use the PNA to control other GPIB instruments, you may want to use COM as the means of talking to the PNA. In GPIB, the PNA can not be configured as both **System Controller** and **talker/listener**. Because the PNA does not support pass control mode, only one mode can be used at a time.
2. If you have legacy code written in SCPI for another network analyzer, you may be able to leverage that code to control the PNA. However, the PNA uses a different platform than previous Agilent Network Analyzers. Therefore, not all commands have a direct replacement. See the PNA [Code Translator Application](#).

## Programming Languages

You can program the PNA with either COM or SCPI using several languages. The most common include:

**Agilent VEE** - With this language you can send text based SCPI commands and also use automation. VEE 6.0 or later is recommended.

**Visual Basic** - This language has great support for automation objects and can be used to drive SCPI commands. The use of VISA drivers for your GPIB hardware interface will make the task of sending SCPI commands easier.

**C++** - This language can do it all. It is not as easy to use as the above two, but more flexible.

## Time Domain

---

Time Domain allows you to view a device response as a function of time. The following are discussed in this topic:

### [Overview](#)

### [How the PNA Measures in the Time Domain](#)

### [Calibration for Time Domain](#)

### [Transmission Measurements](#)

### [Measurement Response Resolution](#)

### [Measurement Range and Alias Responses](#)

### [How to make Time Domain Settings](#)

### [Gating](#)

### [Window Settings](#)

---


**Note:** Time Domain measurements are only available on PNAs with Option 010. See [PNA Options](#)

---

## Overview

In normal operation, the PNA measures the characteristics of a test device as a function of frequency. With Time Domain (opt 010), the frequency information is used to calculate the inverse Fourier transform and display measurements with time as the horizontal display axis. The response values appear separated in time, allowing a different perspective of the test device's performance and limitations.

The graphic below compares the same cable reflection measurement data in both the frequency and time domain. The cable has two bends. Each bend creates a mismatch or change in the line impedance.

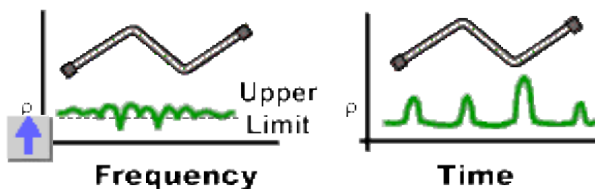


- The frequency domain S11 measurement shows reflections caused by mismatches in the cable. It is impossible to determine where the mismatches physically occur in the cable.
- The time domain response shows both the location and the magnitude of each mismatch. The responses indicate that the second cable bend is the location of a significant mismatch. This mismatch can be [gated out](#), allowing you to view the frequency domain response as if the mismatch were not present. Distance Markers can be used to pinpoint the distance of the mismatch from the reference plane.

## How the PNA Measures in the Time Domain

Time domain transform mode simulates traditional Time-Domain Reflectometry (TDR), which launches an impulse or step signal into the test device and displays the reflected energy on the TDR screen. By analyzing the magnitude, duration, and shape of the reflected waveform, you can determine the nature of the impedance variation in the test device.


The PNA does not launch an actual incident impulse or step. Instead, a Fourier Transform algorithm is used to calculate time information from the frequency measurements. The following shows how this occurs.

A single frequency in the time domain appears as a sine wave. In the following graphic, as we add the fundamental frequency ( $F_0$ ), the first harmonic ( $2F_0$ ), and then the second harmonic ( $3F_0$ ), we can see a pulse taking shape in the Sum waveform. If we were to add more frequency components, the pulse would become sharper and narrower. When the PNA sends discrete frequencies to the test device, it is in effect, sending individual spectral pieces of a pulse separately to stimulate the test device.

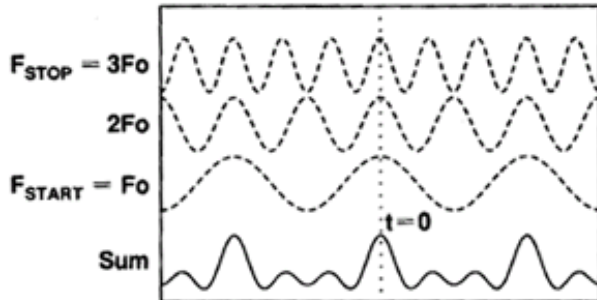


During an S11 reflection measurement, these incident signals reflect from the test device and are measured at the A receiver. This is when the time domain transform calculations are used to add the separate spectral pieces together.

For example, consider a short length of cable terminated with an open. All of the power in the incident signal is reflected, and the reflections are 'in-phase' with the incident signal. Each frequency component is added together, and we see the same pattern as the simulated incident would have looked (above). The magnitude of the reflection is related to the impedance mismatch and the delay is proportional to the distance to the mismatch. The x-axis (time) scale is changed from the above graphic to better show the delay.

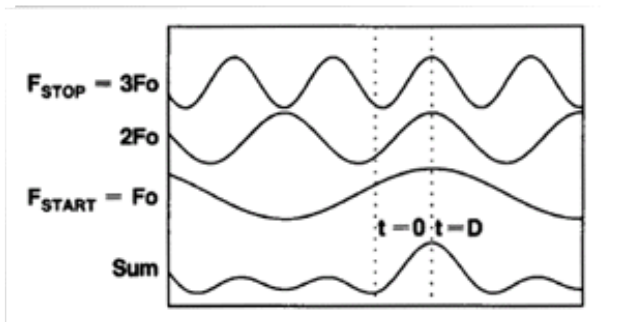

Alternately, the same cable terminated with a short also reflects all of the incident power, but with a phase shift of 180 degrees. As the frequency components from the reflection are added together, the sum appears as a negative impulse delayed in time.

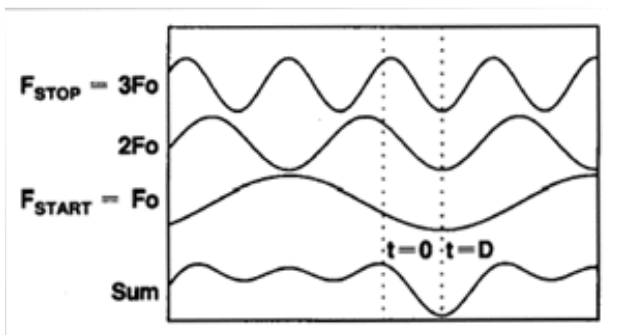

## Calibration for Time Domain

For simplicity, we have discussed incident signals reflecting off discontinuities in the test device. By far the most common network analyzer measurement to transform to time domain is a ratioed S11 measurement. An S11



reflection measurement does not simply display the reflections measured at the A receiver - it displays the ratio (or difference) of the A receiver to the Reference receiver. In addition, the S11 measurement can also be calibrated to remove systematic errors from the ratioed measurement. This is critical in the time domain as the measurement plane, the point of calibration, becomes zero on the X-axis time scale. All time and distance data is presented in reference to this point. As a result, both magnitude and time data are calibrated and very accurate.

The following shows where the time domain transform occurs in the PNA data flow: (see [Data Access Map](#))


1. Acquire raw receiver (A and R1) data
2. Perform ratio (A/R1)
3. Apply calibration
4. Transform data to time domain
5. Display results

Therefore, although a time domain trace may be displayed, a calibration is always performed and applied to the frequency domain measurement which is not displayed.

## Transmission Measurements

The most common type of measurement to transform is an S11 reflection measurement. However, useful information can be gained about a test device from a transformed S21 transmission measurement. The frequency components pass through the test device and are measured at the B receiver. If there is more than one path through the device, they would appear as various pulses separated in time.

For example, the following transmission measurement shows multiple paths of travel within a Surface Acoustic Wave (SAW) filter. The largest pulse (close to zero time) represents the propagation time of the shortest path through the device. It may not be the largest pulse or represent the desired path. Each subsequent pulse represents another possible path from input to output.

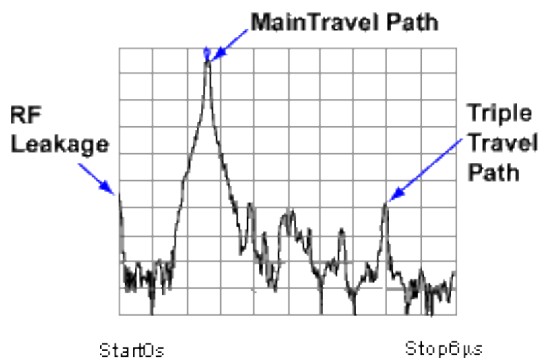

Triple travel is a term used to describe the reflected signal off the output, reflected again off the input, then finally reappearing at the output. This is best seen in a time domain S21 measurement.

## Measurement Response Resolution

In the previous paragraphs, we have seen that using more frequency components causes the assembled waveform to show more detail. This is known as measurement response resolution, which is defined as the ability to distinguish between two closely spaced responses. The following settings also improve measurement response resolution.

---


Note: Adjusting the transform time settings improves **display** resolution, but not measurement resolution.

## Window Settings

### Time Domain Mode

#### **F**requency Span

The following graphic shows the effect of both a narrow and wide frequency span on the response resolution. The wider frequency span enables the analyzer to resolve the two connectors into separate, distinct responses.

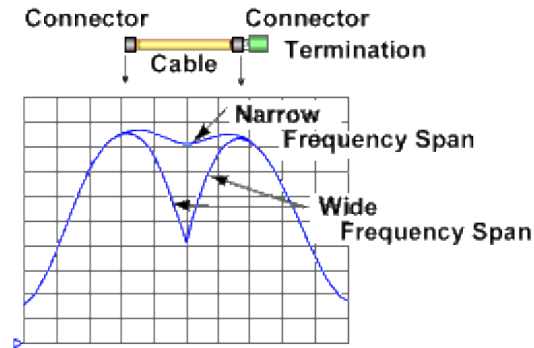

Although a wider frequency span causes better measurement resolution, the measurement range becomes limited. Increasing the frequency range can cause a measurement calibration to become invalid. Be sure to adjust the frequency span BEFORE performing a calibration.

#### **Resolution Formula**

You can calculate the ability of the PNA to resolve two closely spaced responses (in meters) using the following formula:

$$\text{Resolution} = (V_f * c * (\text{points}-1)) / (2 * F_{\text{span}} * N_s)$$

Where:

$V_f$  = Velocity Factor

$c$  = velocity of light in a vacuum ( $2.99796 \times 10^8$  m/sec)

points = number of measurement points

$F_{\text{span}}$  = measurement frequency span

$N_s$  = Sampling factor (**128** for 101 points; **256** for 201 points; **512** for 401 points)

#### **Measurement Range and Alias Responses**

Measurement range is the length in time in which true time domain responses can be seen. The measurement range should be large enough to see the entire test device response without encountering a repetition (alias) of the response. An alias response can hide a true time domain response.

To increase measurement range in both modes, change either of these settings:

- Increase the number of points
- Decrease the frequency span

#### **Notes:**


- After making these settings, you may need to adjust the transform time settings to see the new measurement range.

- Decreasing the frequency span degrades measurement resolution.
- Make frequency span and number of points settings BEFORE calibrating.
- Maximum range also depends on loss through the test device. If the returning signal is too small to measure, the range is limited regardless of the frequency span.

### Alias Responses

An alias response is not a true device response. An alias response repeats because each time domain waveform has many periods and repeats with time (see How the PNA Measures in the Time Domain). Alias responses occur at time intervals that are equal to 1/ frequency step size.

The PNA adjusts the transform time settings so that you should only see one alias free range on either side (positive and negative) of zero time. However, these settings are updated only when one of the toolbar settings are changed.

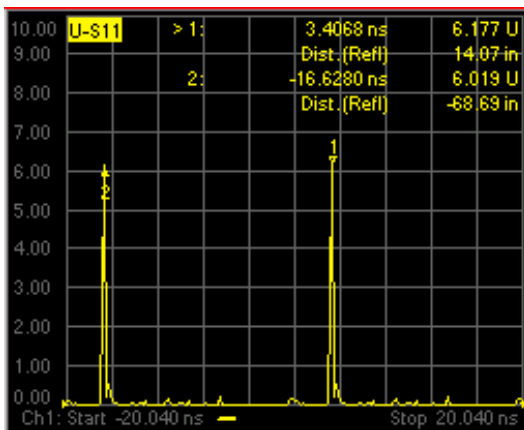

To determine if a response is true, put a marker on the response and change the frequency span. A true device response will not move in time. An alias response will move.

For example, in the above graphic, the marker 1 response occurs at 14.07 inches. When the frequency span is changed, this response remains at 14.07 inches. The marker 2 response moves.

### Range Formula

You can calculate the alias-free measurement range (in meters) of the PNA using the following formula:

$$\text{Range} = V_f * c * (\text{points}-1) / (2 * F_{\text{span}})$$

Where:


$V_f$  = Velocity Factor

$c$  = velocity of light in a vacuum ( $2.99796 \times 10^8$  m/sec)

points = number of measurement points

$F_{\text{span}}$  = measurement frequency span

## How to make Time Domain Settings

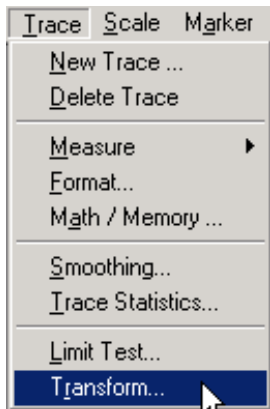


This launches the [Time Domain toolbar](#)



On the toolbar, click **More...** to launch the Time Domain dialog box

Learn more about using the [front panel interface](#)

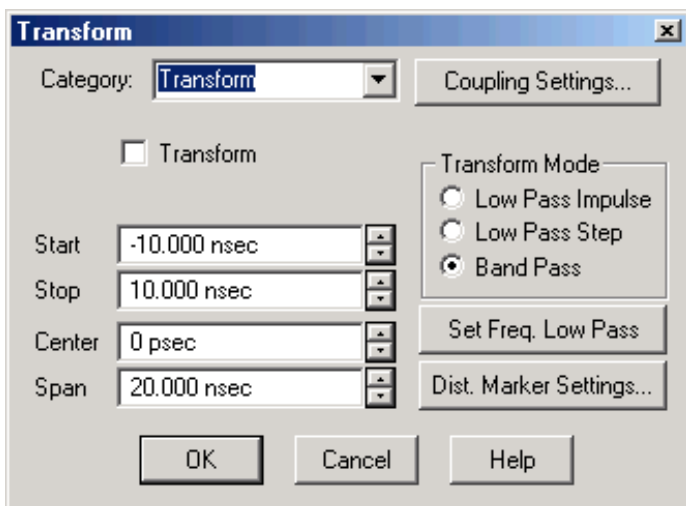

## Transform dialog box help

**Category** Select Transform, Window, or Gating

**Transform** Turns time domain transform ON and OFF.

**Coupling Settings** Launches the [Trace Coupling Settings](#) dialog box.

### Time Settings

The following settings adjust the **display resolution**, allowing you to zoom IN or OUT on a response. They do NOT adjust [measurement range](#) or [measurement resolution](#).

These settings automatically update (when one of these values are updated) to limit the display to one [alias-free response](#) on either side of zero time.

**Start** Sets the transform start time that is displayed on the PNA screen.

**Note:** Zero (0) seconds is always the [measurement reference plane](#). Negative values are useful if moving the reference plane.

**Stop** Sets the transform stop time that is displayed on the PNA screen.

**Center** Sets the transform center time that is displayed in the center of the PNA screen.













**Span** Sets the transform span time that is split on either side of the Center value.

### Transform Mode

Transform modes are three variations on how the time domain transform algorithm is applied to the frequency domain measurement. Each method has a unique application.

| Mode                     | Benefit - application                                                                                                                           | Limitation                                                                                                                                                                                                                                                                                                        |
|--------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Low pass Impulse</b>  | Highest resolution.<br>Most useful for seeing small responses in devices that pass low frequencies, such as cables.                             | In both Low pass modes, frequencies down to DC and negative frequencies are extrapolated. Therefore, the Start frequency is adjusted when you click <u>Set Freq.Low Pass</u><br><br>Because this will affect calibration accuracy, be sure to calibrate AFTER completely setting up your time domain measurement. |
| <b>Low pass Step</b>     | Easiest to identify inductive and capacitive discontinuities in devices that pass low frequencies, such as cables.                              |                                                                                                                                                                                                                                                                                                                   |
| <b>Band pass Impulse</b> | Easiest method - can be used with any frequency sweep.<br>Most useful for measuring band limited devices such as filters and DC blocked cables. | Does NOT show capacitive and inductive reactance<br><br>For the same frequency span and number of points, band pass mode has twice the impulse width, which hides closely spaced responses degrading the response resolution.                                                                                     |

The following chart shows how to interpret results from various discontinuity impedances using Low pass Step and either Low pass or Band pass Impulse modes.

| IMPEDANCE             | STEP RESPONSE                                                                                                 | IMPULSE RESPONSE                                                                                              |
|-----------------------|---------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------|
| OPEN                  | <br>Unity Reflection       | <br>Unity Reflection       |
| SHORT                 | <br>Unity Reflection = 180 | <br>Unity Reflection = 180 |
| RESISTOR<br>$R > Z_0$ |                            |                            |
| RESISTOR<br>$R < Z_0$ |                            |                            |
| INDUCTOR              |                            |                            |
| CAPACITOR             |                            |                            |

### Effect on Measurement Range

**Band pass mode** - measurement range is inversely proportional to frequency step size.

**Low pass mode** - measurement range is inversely proportional to the fundamental (start ) frequency AFTER clicking Set Freq. Low Pass.

**Set Freq. Low Pass** USE ONLY IN LOW PASS MODES

Recomputes the start frequency and step frequencies to be harmonics of the start frequency. Start frequency is computed by the following formula: **Low Pass Start Frequency = Stop Frequency / Number of points.**

The computed value must always be greater than or equal to the analyzer's minimum frequency.

---

**Note:** The number of points or stop frequency may be changed in order to compute this value.

---

**Distance Marker Settings** Launches the Distance Marker Settings dialog box.

## Gating

Perhaps the most beneficial feature of time domain transform is the Gating function. When viewing the time domain response of a device, the gating function can be used to "virtually" remove undesired responses. You can then simultaneously view a frequency domain trace as if the undesired response did not exist. This allows you to characterize devices without the effects of external devices such as connectors or adapters.

---

**Note:** When a discontinuity in a test device reflects energy, that energy will not reach subsequent discontinuities. This can "**MASK**", or hide, the true response which would have occurred if the previous discontinuity were not present. The PNA Gating feature does NOT compensate for this.

---

The following measurements images show a practical example how to use and perform gating. The test device is a 10inch cable, then a 6 dB attenuator, terminated with a short. The following four discontinuities are evident in window 2, from left to right:

1. A discontinuity in the test system cable which appeared after calibration. It is identified by marker 2 at -10.74 inches (behind the reference plane).
2. A discontinuity in the 10 inch device cable shortly after the reference plane.
3. The largest discontinuity is the attenuator and short shown by marker 1 at -12.67 dB ( 6 dB loss in both forward and reverse direction).
4. The last discontinuity is a re-reflection from the device cable.


We will gate IN the attenuator response. All other responses will be gated OUT.

**Window 1.** Create original S11 frequency domain trace. Shows ripple from all of the reflections.


**Window 2.** Create a new S11 trace - same channel; new window. Turn Transform ON.

**Window 3.** On the transformed trace, turn gating ON. Center the gate on the large discontinuity (2.500ns). Adjust gate span to completely cover the discontinuity. Select Bandpass gating type.

**Window 4.** On the original frequency measurement, turn Gating ON (Transform remains OFF). View the measurement without the effects of the two unwanted discontinuities. The blue trace is a measurement of the 6 dB attenuator with the unwanted discontinuities PHYSICALLY removed. The difference between the two traces in window 4 is the effect of "masking".

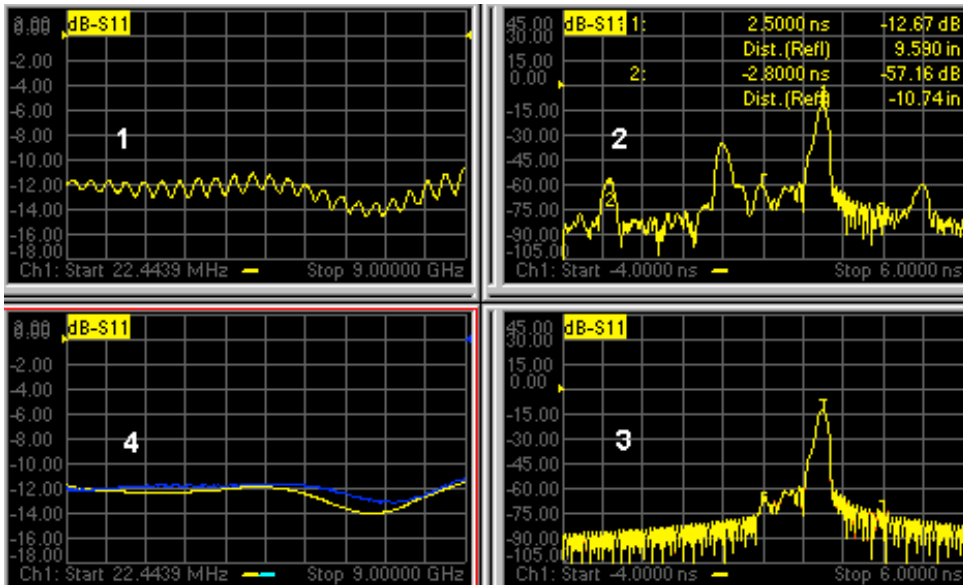

Learn how to launch the Transform dialog box

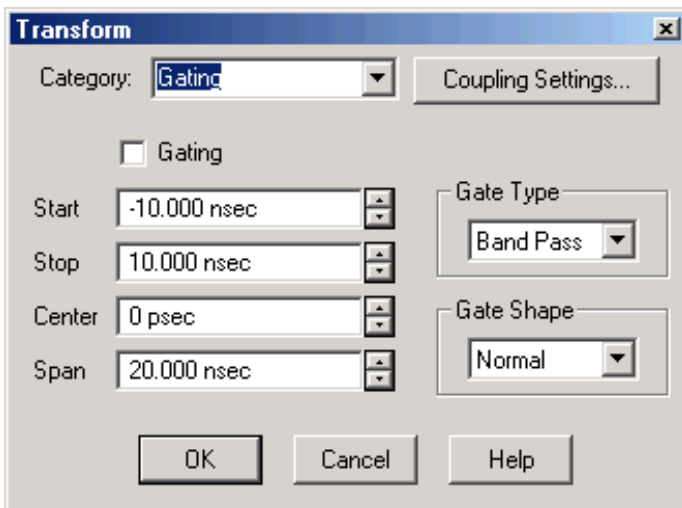

### Transform Gating dialog box help

**Gating** Turns Gating ON and OFF.

**Coupling Settings** Launches the [Setup Trace Coupling](#) dialog box.

**Start** Specifies the start time for the gate.

**Stop** Specifies the stop time for the gate.

**Center** Specifies the value at the center of the area that is affected by the gating function. This value can be anywhere in the analyzer range.


**Span** Specifies the range to either side of the center value of area that is affected by the gating function.

**Gate Type** Defines the type of filtering that will be performed for the gating function. The gate start and stop flags on the display point toward the part of the trace you want to keep.

- **Bandpass** - KEEPS the responses within the gate span.
- **Notch** - REMOVES the responses with the gate span.

**Gate Shape** Defines the filter characteristics of the gate function. Choose from Minimum, Normal, Wide,

Maximum

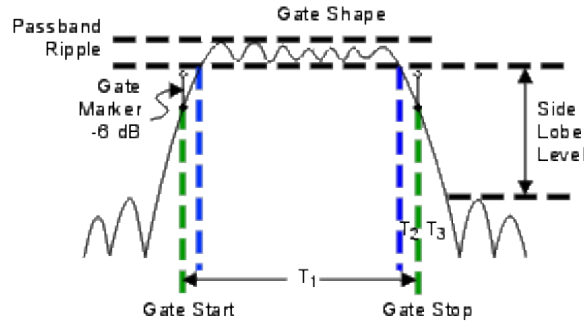

| Gate Shape | Passband Ripple | Sidelobe Levels | Cutoff Time    | Minimum Gate Span |
|------------|-----------------|-----------------|----------------|-------------------|
| Minimum    | ±0.1 dB         | -48 dB          | 1.4/Freq Span  | 2.8/Freq Span     |
| Normal     | ±0.1 dB         | -68 dB          | 2.8/Freq Span  | 5.6/Freq Span     |
| Wide       | ±0.1 dB         | -57 dB          | 4.4/Freq Span  | 8.8/Freq Span     |
| Maximum    | ±0.01 dB        | -70 dB          | 12.7/Freq Span | 25.4/Freq Span    |

**Cutoff time** -- is the time between the stop time (-6 dB on the filter skirt) and the peak of the first sidelobe. The diagram below shows the overall gate shape and lists the characteristics for each gate shape.

- T<sub>1</sub> is the gate span, which is equal to the stop time minus the start time.
- T<sub>2</sub> is the time between the edge of the passband and the 6 dB point, representing the cutoff rate of the filter.
- T<sub>3</sub> is the time between the 6 dB point and the edge of the gate stopband.
- For all filter shapes T<sub>2</sub> is equal to T<sub>3</sub>, and the filter is the same on both sides of the center time.

**Minimum gate span** -- is twice the cutoff time. Each gate shape has a minimum recommended gate span for proper operation. This is a consequence of the finite cutoff rate of the gate. If you specify a gate span that is smaller than the minimum span, the response will show the following effects:

- distorted gate shape that has no passband
- distorted shape
- incorrect indications of start and stop times
- may have increased sidelobe levels


### Window Settings

There are abrupt transitions in a frequency domain measurement at the start and stop frequencies, causing overshoot and ringing in a time domain response. The window feature is helpful in lessening the abruptness of the frequency domain transitions. This causes you to make a tradeoff in the time domain response. Choose between the following:


- **Minimum Window = Better Response Resolution** - the ability resolve between two closely spaced responses.



- **Maximum Window = Dynamic Range** - the ability to measure low-level responses.

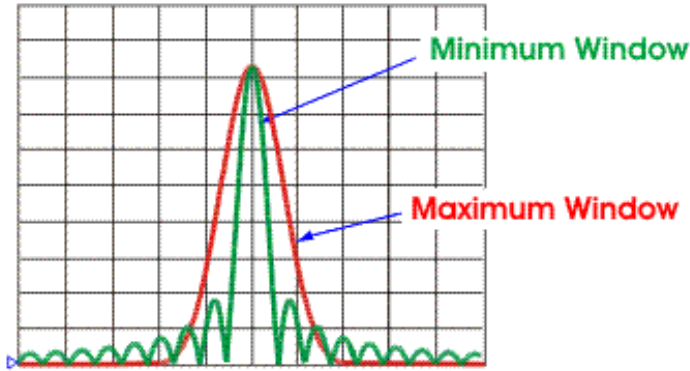

Learn how to launch the Transform dialog box

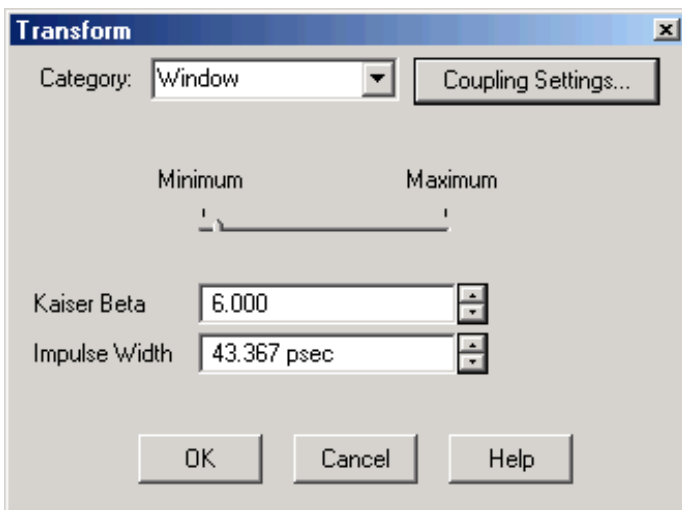

### Transform - Window dialog box help

**Coupling Settings** Launches the [Setup Trace Coupling](#) dialog box.

The window settings balance response resolution versus dynamic range.

- Minimum Window = Best Response Resolution
- Maximum Window = Best Dynamic Range

The following three methods all the set window size. For best results, view the time domain response while making these settings.

- **Minimum - Maximum** Move the slider with a mouse to change the window size
- **Kaiser Beta** Changes window size using a Kaiser Beta value
- **Impulse Width** Changes window size using an Impulse Width value


Learn more about [Windowing](#) (top)

## How to make Trace Coupling Settings

You can launch the **Trace Coupling Settings** dialog box from any of the following dialog boxes:

- [Transform](#)
- [Gating](#)
- [Window](#)

Learn more about using the [front panel interface](#)

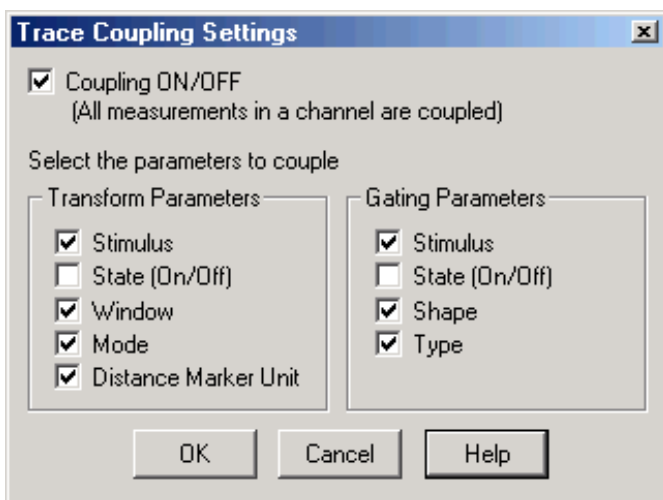

## Trace Coupling Settings dialog box help

Trace coupling allows you to change time domain parameters on a measurement, and have the same changes occur for all other measurements in the channel.

For example:

If you are simultaneously viewing a frequency domain measurement and time domain measurement,  
and **Coupling** is enabled in this dialog box,  
and ALL **Gating Parameters** are checked in this dialog box,  
and on the time domain measurement you change the **Gate Span** parameter,

Then the frequency domain measurement will automatically change to reflect the time domain gated span.

**Coupling ON/OFF** Check to enable coupling. All of the measurements in the active channel are coupled.

The following parameters are available for coupling:

### Transform Parameters

**Stimulus** Start, Stop, Center, and Span TIME settings.

**State (On/Off)** Transform ON and OFF

**Window** Kaiser Beta / Impulse Width

**Mode** Low Pass Impulse, Low Pass Step, Band Pass


### Gating Parameters

**Stimulus** Start, Stop, Center, and Span TIME settings.

**State** (On/Off) Gating ON and OFF

**Shape** Minimum, Normal, Wide, and Maximum

**Type** Bandpass and Notch

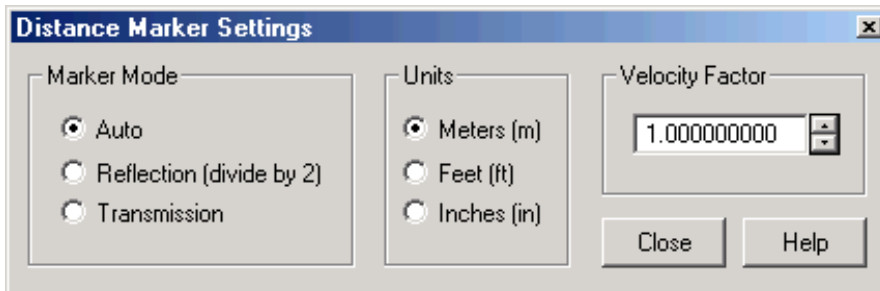

### Distance Marker Settings dialog box help

To launch this dialog box, click **Dist. Marker Settings** on the Transform dialog box.

When markers are present on a time domain measurement, distance is automatically displayed on the marker readout, marker table, and print copy. To learn how to create markers on your measurement see marker settings.

This dialog box allows you to customize the time domain distance marker readings.

These settings affect the display of ALL markers for only the ACTIVE measurement (unless **Distance Marker Unit** is coupled on the Trace Coupling dialog box).

**Marker Mode** Specifies the measurement type in order to determine the correct marker distance.

- Select **Auto** for S-Parameter measurements.
- Select **Reflection** or **Transmission** for arbitrary ratio or unratioed measurements.

**Auto** If the active measurement is an S-Parameter, automatically chooses reflection or transmission. If the active measurement is a non S-Parameter, reflection is chosen.

**Reflection** Displays the distance from the source to the receiver and back divided by two (to compensate for the return trip.)

**Transmission** Displays the distance from the source to the receiver.

**Units** Specifies the unit of measure for the display of marker distance values.

**Velocity Factor** Specifies the numerical value related the speed of energy through transmission lines with different dielectrics. This is useful in Time Domain for accurate display of time and distance markers. Some common values are:

- 0.66 - Polyethylene dielectric cable
- 0.7 - Teflon dielectric
- 1.0 - The speed of light in a vacuum

This setting can also be made from the Electrical Delay and Port Extensions dialog boxes.



## Frequency Offset

---

The PNA Option 080 provides you with the hardware and basic software to make Frequency Offset Measurements. This topic discusses the PNA settings that are relevant to making these types of measurements. See [Frequency Converting Device Measurements](#) for more information on making specific device measurements.

**Note:** The Frequency Converter Application [Option 083](#) simplifies the task of making extremely accurate frequency offset measurements on MOST frequency converting devices.

---

### [Frequency Offset Dialog Box](#)


### [Setup Examples](#)

### [Test Set \(Reference Switch\) Dialog Box](#)


#### Other Frequency Offset topics

---

#### How to access the Frequency Offset dialog



Learn more about using the [front panel interface](#)

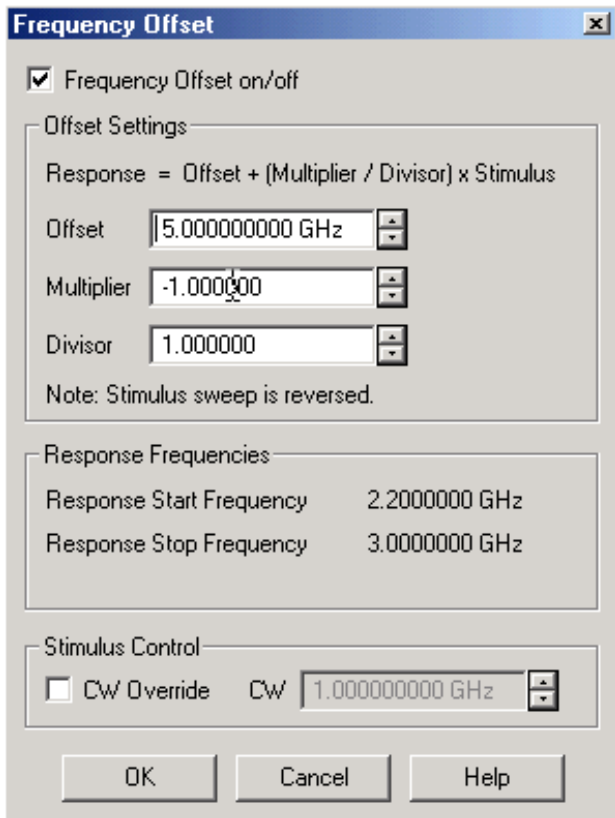

### Frequency Offset dialog box help

**Note:** With basic Frequency Offset measurements, Port 1 or Port 2 can be configured as either the source (stimulus) or receiver (response). This is NOT true with [Option 083](#).

**Frequency Offset on/off** Enables Frequency Offset Mode on ALL measurements that are present in the active channel. This immediately causes the source and receiver to tune to separate frequencies. The receiver frequencies are specified in the remaining settings in this dialog box. To make the stimulus settings, on the **Channel** menu click **Start / Stop**, then **OK**.

**Tip:** To avoid unnecessary errors, first make other settings on this dialog box, then click **Frequency Offset ON**.

#### Offset Settings

The receivers tune to the frequency specified by the following formula:

**Response = Offset +(Multiplier / Divisor) x Stimulus** (or source)

Where:

**Offset** Specifies an absolute offset frequency in Hz. For mixer measurements, this would be the LO frequency. Range is +/- 1000 GHz. Offsets can be positive or negative. [See an example.](#)

**Multiplier** Specifies (along with the divisor) the value to multiply by the stimulus. Range is +/- 1000. Negative multipliers cause the stimulus to sweep in decreasing direction. For mixer measurements, this would be for setups requiring the Input frequency to be less than LO frequency. [See an example.](#)

**Divisor** Specifies (along with the multiplier) the value to multiply the stimulus. Range is 1 to 1000

#### Stimulus CW Override

Use this setting to establish a fixed (CW) stimulus frequency while measuring the Response over a swept frequency range. For example, the PNA stimulus may be applied to the RF input of a mixer whose local oscillator (LO) is being swept. Because the IF output of the mixer will be swept, the PNA receivers must also be swept. [See an example.](#)

To set up such an instrument state:

1. Set the Stimulus Sweep Type (Linear, Log, or Segment Sweep) and frequency settings as well as the Offset, Multiplier and Divisor to cause the desired Response Start and Stop frequencies.
2. Turn ON Frequency Offset - the receivers will now sweep over the desired frequencies.
3. Turn ON CW Override and set the desired CW frequency for the source.

#### Notes:

When Frequency Offset is enabled, ALL receivers on the channel tune to the offset frequency, including the reference receiver. Therefore S21 (conversion loss) measurements will not display the response frequency relative to the input frequency.

If you want to measure and display measurements at both the stimulus and response frequencies, you must use two channels. These types of ratioed measurements must be computed external to the PNA.

To calibrate for frequency offset measurements, see..[Frequency Offset Calibration](#).

#### Using Power Sweep for Testing Mixers

To measure the gain compression of a mixer, you need to sweep the input power to the mixer. The input and output frequencies are fixed but offset from one another. To set the input and output frequencies of the mixer under test:

1. On the PNA menu, click **Sweep**, then **Sweep Type**. Select **Power Sweep**. Also, set the CW (input) frequency of the mixer under test.
2. Click **Channel**, then **Frequency Offset**. Set **Offset** to reflect the appropriate LO and response of the mixer under test.

#### Setup Examples

1. **Swept Stimulus** (1000 MHz to 1100 MHz)  
**Swept Response** (2500 MHz to 2700 MHz)

Make the following settings:

On the **Channel** menu click **Start / Stop**

Start Frequency = 1000 MHz

Stop Frequency = 1100 MHz

In the **Frequency Offset** dialog:

Offset = 500 MHz

Multiplier = 2

Divisor = 1

Frequency Offset = ON

The above settings cause the following response frequencies:

Response = Offset + (Multiplier / Divisor) x Stimulus

Response Start Frequency = 500 + [(2 / 1) \* 1000]  
= 2500 MHz

Response Stop Frequency = 500 + [(2 / 1) \* 1100]  
= 2700 MHz

2. **Fixed Stimulus** (1000 MHz)

**Swept Response** (2500 MHz to 2700 MHz)

Make the following settings:

On the **Channel** menu click **Start / Stop**

Start Frequency = 2500 MHz

Stop Frequency = 2700 MHz

In the **Frequency Offset** dialog:

Stimulus CW Override: ON

CW Frequency: 1000 MHz

Offset = 0 MHz

Multiplier = 1

Divisor = 1

Frequency Offset = ON

---

3. **Swept Stimulus** (1000 MHz to 1100 MHz)

**Fixed Response** (2500 MHz)

Make the following settings:

On the **Channel** menu click **Start / Stop**

Start Frequency = 1000 MHz

Stop Frequency = 1100 MHz

In the **Frequency Offset** dialog:

Offset = 2500 MHz

Multiplier = 0

Divisor = 1

Frequency Offset = ON

The above settings cause the following response frequencies:

Response = Offset + (Multiplier / Divisor) x Stimulus

Response Start Frequency =  $2500 + [(0 / 1) * 1000]$   
= 2500 MHz

Response Stop Frequency =  $2500 + [(0 / 1) * 1100]$   
= 2500 MHz

---



4. **Swept Stimulus** (2500 MHz to 2600 MHz)  
**Swept Response** (1000 MHz to 1100 MHz)  
**External LO** (not supplied): 1500 MHz

Start Frequency = 2500 MHz

Stop Frequency = 2600 MHz

In the **Frequency Offset** dialog:

Offset = -1500 MHz

Multiplier = 1

Divisor = 1

Frequency Offset = ON

The above settings cause the following response frequencies:

Response = Offset + (Multiplier / Divisor) x Stimulus

Response Start Frequency =  $-1500 + [(1 / 1) * 2500]$   
= 1000 MHz

Response Stop Frequency =  $-1500 + [(1 / 1) * 2600]$   
= 1100 MHz

5. **Swept DECREASING Stimulus** (1100 MHz to 1000 MHz)  
**Swept INCREASING Response** (1400 MHz to 1500 MHz)

**External LO** (not supplied): 2500 MHz

For some frequency-translating devices, as the input frequency increases, the output frequency decreases. The PNA can only display the response (output) as increasing. Therefore, the same effect can be obtained by sweeping the stimulus decreasing from higher to lower frequency. This causes an increasing response to be measured and displayed.

To accomplish this, set the multiplier to a negative value. This causes the PNA source to automatically sweep in reverse; from the higher frequency to the lower frequency.

Make the following settings:

On the **Channel** menu click **Start / Stop**

Start Frequency = 1000 MHz

Stop Frequency = 1100 MHz

In the **Frequency Offset** dialog:

Offset = 2500 MHz

Multiplier = -1

Divisor = 1

Frequency Offset = ON

The above settings cause the following response frequencies:

Response = Offset + (Multiplier / Divisor) x Stimulus

Response Start Frequency =  $2500 + [(-1 / 1) * 1000]$   
= 1500 MHz

Response Stop Frequency =  $2500 + [(-1 / 1) * 1100]$   
= 1400 MHz

The response cannot sweep backwards, so the PNA reverses the stimulus frequencies.

Stimulus Start Frequency = 1100 MHz

Stimulus Stop Frequency = 1000 MHz

Response Start Frequency = 1400 MHz


Response Stop Frequency = 1500 MHz

## Test Set Reference Switch


PNA models with [option 081](#) have a switch in the test set that allows you to bypass the port 1 reference receiver through the front panel Reference 1 connectors. This switch lets you easily switch between standard S-Parameter measurements and measurements using a reference mixer. You could use this feature to make standard S11 measurements and converter transmission measurements relative to a reference ("golden") mixer.

**Note:** The Frequency Converter Application [Option 083](#) simplifies the task of making extremely accurate phase measurements on MOST frequency converting devices.

### How to access the Test Set dialog box

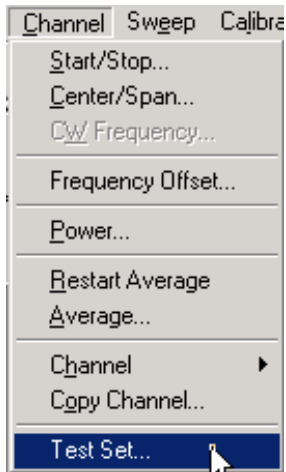

Learn more about using the [front panel interface](#)

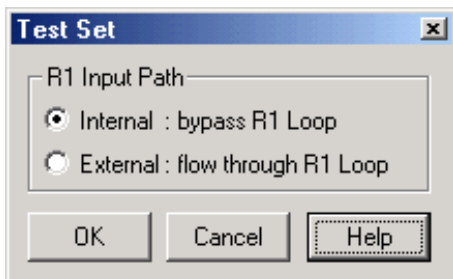

## Test Set dialog box help

**Note:** This feature is only available on PNA models with Option 081 - external reference switch.

### R1 Input Path

**Internal: bypass R1 Loop** Connects the port 1 source directly to the R1 receiver.

**External: flow through R1 Loop** Allows direct access to the R1 receiver through the Reference 1 front-panel connectors.

See block diagram of reference switch.

## Frequency Converting Device Measurements

---

Many frequency offset measurements can be made using the PNA with option 080. The following is a list of some of those measurements and how they are made.

[Conversion Loss](#)

[Conversion Compression](#)

[Return Loss and VSWR](#)

[Isolation](#)

[Harmonic Distortion](#)

See Also: [Frequency Offset Measurement Accuracy](#)

## Frequency Offset Measurement Accuracy

---

This topic discuss methods that can be used to make accurate frequency offset measurements.

### Calibrations

### Mismatch Errors

### Accurate and Stable LO

**See other Mixer Measurement topics**

## Calibrations

With Frequency Offset measurements, the stimulus and response frequencies are different. Standard calibration error terms are calculated using reference measurements. Therefore, traditional calibration methods such as full 2-port SOLT cannot be used with frequency offset.

Frequency Converter Application (option 083) offers fully calibrated scalar and phase frequency offset measurements.

If you do not have option 083, Source and Receiver Power calibrations can be used to calibrate your Frequency Offset measurements.

### Source Power calibration:

- Sets accurate power level at stimulus frequencies regardless of the receiver that will be used in the measurement.
- Can be copied to other channels with copy channels feature.
- Can be interpolated.

### Receiver Power Cal:

- Requires a source cal to have already been performed and applied.
- Cannot be copied to other channels.

### Therefore:

- Start by performing a source power cal over the combined stimulus and response frequencies.
- Copy the channel to other needed channels and the source power cal is copied.
- Change the frequency range of the copied channel to response frequency
- Perform a receiver cal at the response frequencies on individual channels.
- Change the frequency range to stimulus frequency and switch frequency offset ON.
- On Status Bar, ensure that source and receiver cals are ON (source cal will be interpolated).

See [Conversion Loss Measurements](#) for an example.

Learn more about [source and receiver power calibrations](#).

## Mismatch Errors


Mismatch errors result when there is a connection between two ports that have different impedances. With S-parameter measurements, these mismatches are measured and mathematically removed during a full 2-port calibration. This is much more difficult with frequency offset measurements. A much easier solution is to use high-quality attenuators on the input and output of the mixer.

By adding a high-quality attenuator to a port, the effective port match can be improved by up to twice the value of the attenuation. For example, a 10-dB attenuator, with a port match of 32 dB, can transform an original port match of 10 dB into an effective match of 25 dB. However, as the match of the attenuator approaches the match of the original source, the improvement diminishes.


---

**Note:** The Frequency Converter Application (option 083) uses calibration techniques that correct for mismatch errors.

---

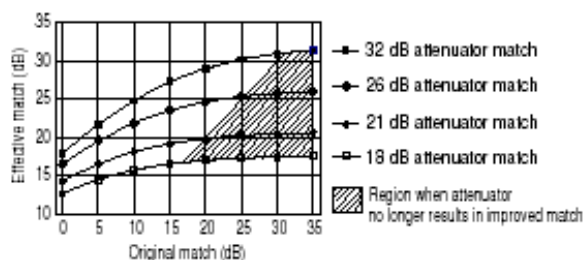

The larger the attenuation, the more nearly the resulting match approaches that of the attenuator, as shown in the following graphic. However, excessive attenuation is not desired because that will decrease the dynamic range of the measurement system.

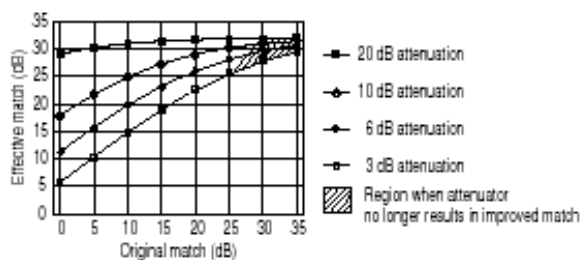

## Accurate and Stable LO

When using frequency offset mode, if the LO signal is not accurate and stable, the output signal will not be at the expected response frequency. As a result, the output signal can fall on the skirts of the PNA receiver IF filter, or fall completely outside of the receiver filter passband.

Also, the LO power level is critical in mixer measurements. Be sure to monitor these power levels closely.

## Conversion Loss (or Gain)

---

### What is Conversion Loss?


### Why Measure Conversion Loss?

### How to Measure Conversion Loss

[See other Frequency Converting Device Measurements](#)

## What is Conversion Loss?

Conversion loss is defined as the ratio of the power at the output frequency to the power at the input frequency with a given LO (local oscillator) power. This is illustrated in the graphic below. A specified LO power is necessary because conversion loss varies with the level of the LO, as the impedance of the mixer diode changes.

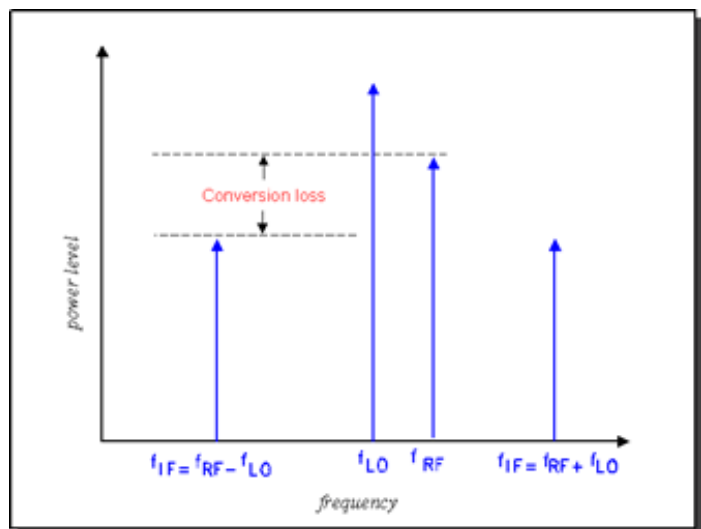

## Why Measure Conversion Loss?


Conversion loss (or gain in the case of many converters and tuners) is a measure of how efficiently a mixer converts energy from the input frequency to the output frequency. If the conversion loss response of a mixer or converter is not flat over the frequency span of intended operation, valuable information may be lost from the resulting output signal.

## How to Measure Conversion Loss

Conversion loss is a transmission measurement. It is measured by applying an input signal (stimulus) and an LO signal at specific known power levels, and measuring the resulting output signal level. Because the output frequency is different from the input frequency, frequency offset mode (option 080) must be used for this measurement.

**Note:** This measurement is made much easier if your PNA has the Frequency Converter Application

## Equipment Setup

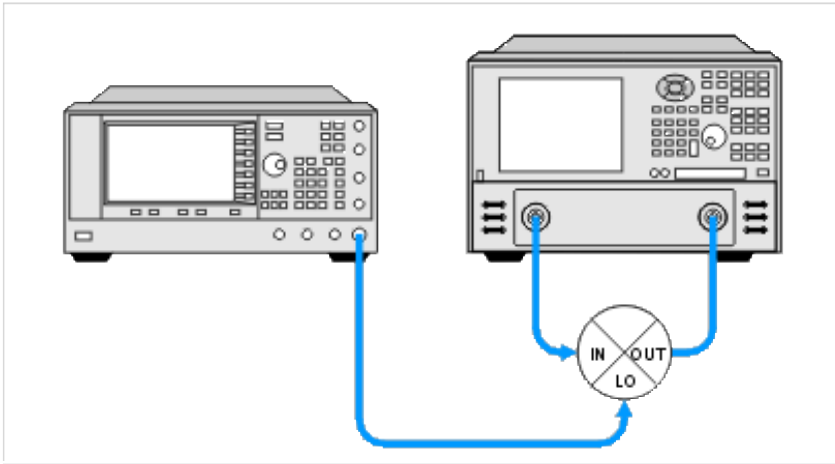

### Example: A calibrated Conversion Loss (Down-converter) measurement

#### Swept Input with Fixed LO = Swept Output

- RF Input: 3.1 - 3.3 GHz
- LO: 2.2 GHz
- IF Output: 900 - 1100 MHz

#### PNA setup and calibrate on channel 1

- On channel 1 create an unratioed R measurement over the ENTIRE input and output frequency span (.9 - 3.3 GHz). This will be the base source power cal that will be copied to the R and B channel measurements.
- Perform a source calibration using a power meter. This makes the power level at the input of the mixer very accurate.

#### Setup Reference measurement on channel 2

- Copy channel 1 to channel 2 which will display the reference input to the mixer. The channel 1 source power cal is copied with the other channel settings.
- Change measurement to R1 unratioed.
- Change RF Input frequency to 3.1 - 3.3 GHz. The source power cal becomes interpolated.
- Perform receiver power cal. Do not need to make physical connections. The PNA source is internally connected to the R1 receiver. Makes the R receiver read the source power level.

#### Setup B measurement on channel 3

- Copy channel 1 to channel 3. This channel will display the output of the mixer. The channel 1 source power cal is copied with the other channel settings.
- Change measurement to B unratioed.
- Change IF Output frequency to .9 - 1.1 GHz. This causes the source power cal becomes interpolated.



- Connect thru line from port 1 to port 2.
- Perform receiver power cal. This makes the B receiver read the source power at the IF Output frequencies.
- Turn OFF receiver power cal. This prevents an error when changing to input frequencies (next step).
- Change RF Input frequency to 3.1 - 3.3 GHz. This changes the channel back to the mixer RF Input frequencies.
- Enable Frequency Offset.
- Change Offset to (-2.2 GHz). This tunes the B receiver to the IF Output frequencies .9 to 1.1 GHz. **Note:** The minus sign indicates a down-converter measurement.
- Turn ON receiver power cal.


### Measure the Mixer

- Connect the mixer.
- Adjust scaling to suit your needs.
- Enable markers to read power levels for each trace.

The display below shows:

- Ch3 B receiver (bottom trace) absolute output power.
- Ch2 R1 receiver measurement (top trace) absolute input power to the mixer.

With this method, the conversion loss math (B/R1) must be performed manually. Markers are set individually for each channel, and trace math is not supported between channels. Also, the B/R1 ratio measurement is not supported with receiver power Cal turned on. However, conversion loss (C21) measurements can be made directly and are much easier using the Frequency Converter Application, FCA (Opt 083).

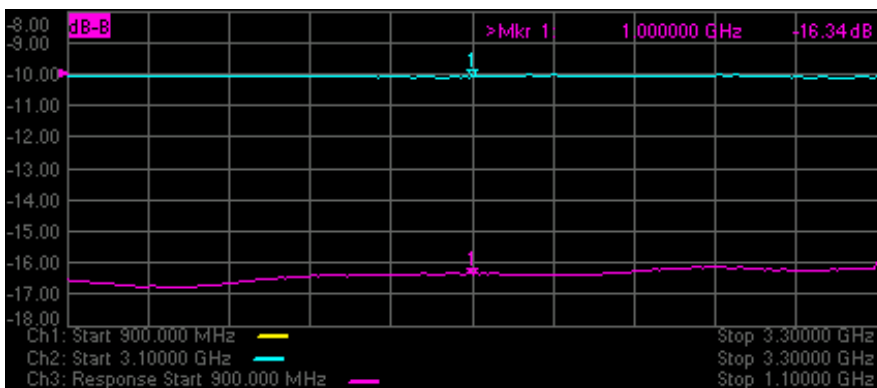

## Conversion Compression

---

### What is Conversion Compression?

### Why Measure Conversion Compression?

### How to Measure Conversion Compression


### Measurement Accuracy Considerations

### See other Frequency Converting Device Measurements

## What is Conversion Compression?

Conversion compression is a measure of the maximum input signal level for which a mixer will produce linear operation. It is very similar to the gain compression experienced in amplifiers.

To understand conversion compression, you must first understand conversion loss. This is the ratio of the mixer output level to the mixer input level. This value remains constant over a specified input power range. When the input power level exceeds a certain maximum level, the constant ratio between input and output power levels begins to change. The point at which the ratio has decreased 1 dB is called the 1-dB compression point. This is illustrated in the graphic below.

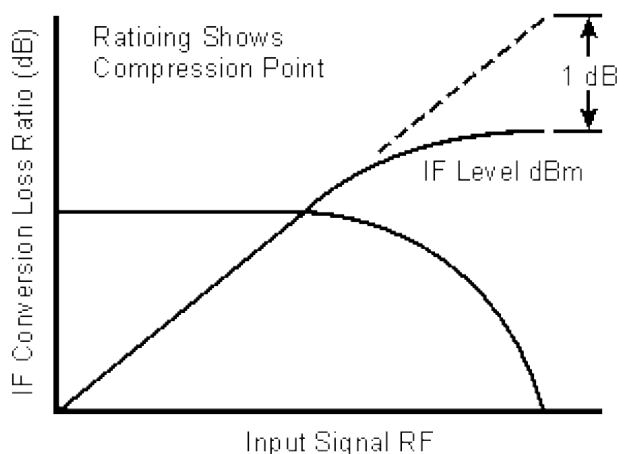


## Why Measure Conversion Compression?

Conversion compression is an indicator of the dynamic range of a device. Dynamic range is generally defined as the difference between the noise floor and the 1-dB compression point.

## How to Measure Conversion Compression

The equipment and setup used to measure conversion compression are essentially the same as for measuring conversion loss and is illustrated in the following graphic.

The PNA performs a power sweep using frequency-offset mode and the resulting display shows the mixer's output power as a function of its input power. The 1-dB compression point (or others such as 3-dB) can be determined using markers.

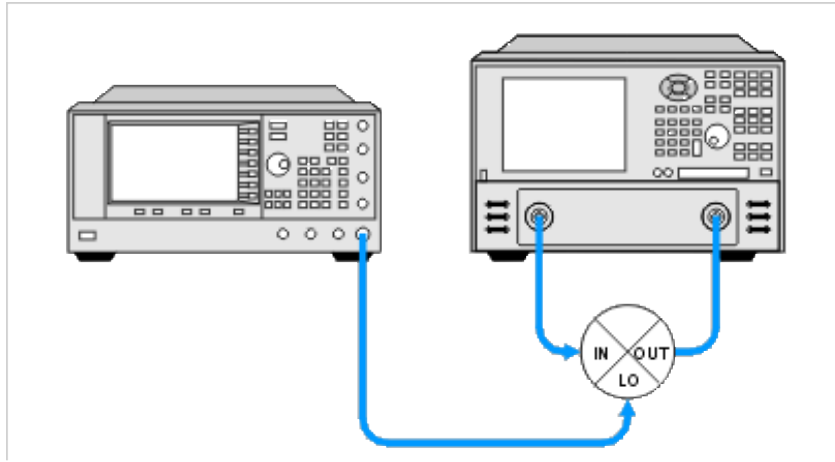

## Measurement Accuracy Considerations

### Equipment Setup Considerations

- The couplers in the PNA have very good directivity. If the return loss of the DUT is bad, the reflected signal gets sampled by the PNA and can result in errors. This relates to error in DUT gain. To increase the accuracy, an attenuator can be added between the PNA's source port and the DUT's input port. Normally a 6- to 10-dB attenuator is sufficient. Addition of this attenuator, however, decreases the available drive to the DUT.
- With high drive levels the PNA can be driven into compression resulting in measurement error. With excessive drive levels, the PNA can be damaged. Add an attenuator between the output of the DUT and the receiver input of the PNA to avoid these problems.

### Calibration Considerations

- Source power calibration can be used to provide a high level of accuracy for this measurement.
- If your PNA has the Frequency Converter Application (option 083), you can perform a Scalar Mixer Calibration to obtain a more accurate measurement.

## Isolation Measurements of Frequency Converting Devices

---

### What is Isolation?

### Why Measure Isolation?

### How to Measure Isolation


[See other Frequency Converting Device Measurements](#)

## What is Isolation?

Isolation is a measure of the leakage, or feedthrough, from one port to another. The more isolation a mixer provides, the lower the amount of feedthrough. Isolation is measured at the same frequency as the stimulus, not the converted or shifted frequency. Therefore, Frequency Offset capability is not necessary for these measurements.

Three main isolation terms are of interest for mixer measurements:

- LO-to-OUT isolation ( $V_{LO}$ )
- LO-to-IN isolation ( $V_{LO}$ )
- IN-to-OUT feedthrough ( $V_{IN}$ )

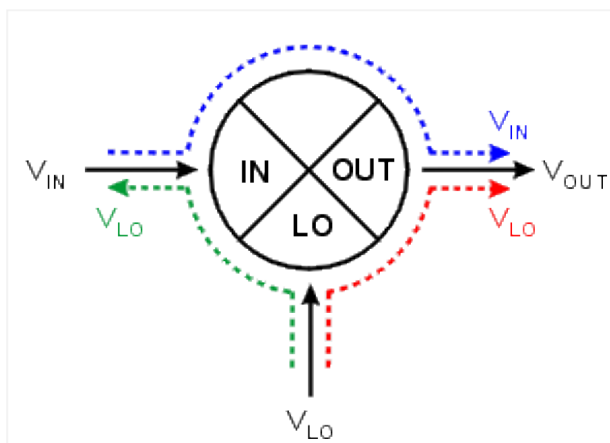

## Why Measure Isolation?

Any unwanted signal "leaking" through the device will mix with the desired output signal creating intermodulation products, adding to intermodulation distortion. These unwanted signals may be difficult to filter out.

## How to Measure Isolation


Use the following setups to measure the isolation of a mixer:

Note the following:


- The Input to Output isolation is very dependent on the LO power level. Isolation should be measured with the LO power at its normal operating level.

- Each of the ports not being tested should be terminated with an impedance typical of actual operation. This may not always be the characteristic impedance,  $Z_0$  (usually 50 or 75 ohms). For example, if the OUT port of a mixer is intended to be directly connected to a filter, then this filter should be used when measuring the LO-to-IN feedthrough.


### LO-TO-IN ISOLATION

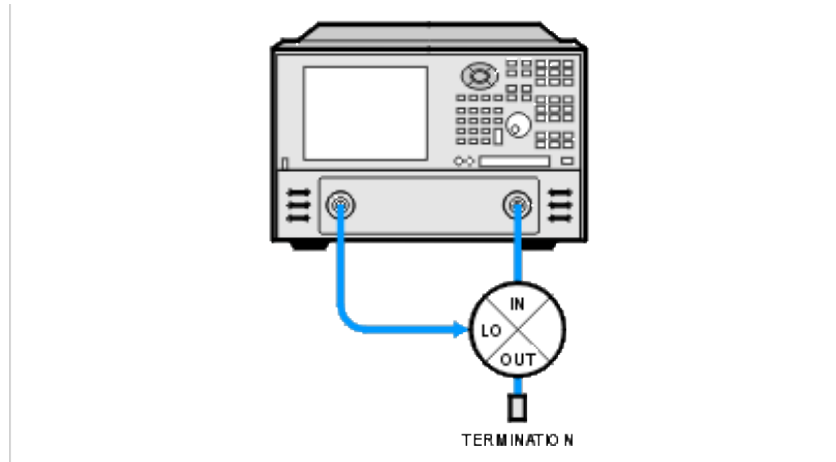

### LO-TO-OUT ISOLATION

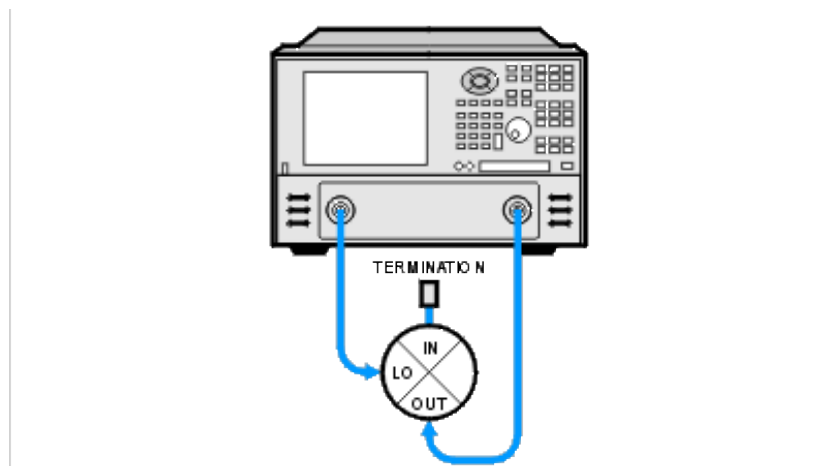

### IN-TO-OUT ISOLATION

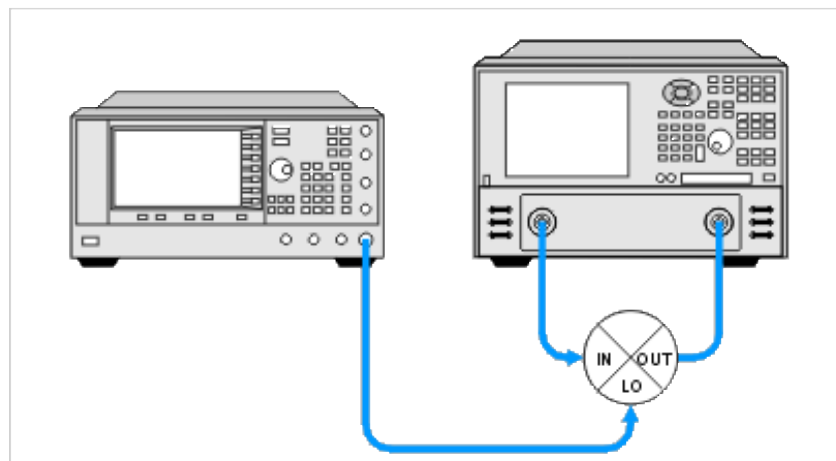

## Measuring Converters vs. Mixers

Measuring IN-to-OUT feedthrough of a converter is identical to that of a mixer. The IN-to-OUT feedthrough is generally very small for a converter due to the inclusion of an IF filter in the device. Because of this, the measurement may require the PNA to have increased dynamic range.

Measuring LO leakage (LO-to-OUT and LO-to-IN) of a converter requires a different technique because the LO port is typically not accessible:

- The PNA can be tuned to the frequency of the LO signal and either the OUT or IN port connected to the PNA receiver port. The PNA source port is not connected.
- A spectrum analyzer can be connected to either the OUT or IN port and tuned to the frequency of the LO signal.

# Harmonic Distortion

---

## What is Harmonic Distortion?

## Why Measure Harmonic Distortion?

## How to Measure Harmonic Distortion

## Measurement and Accuracy Considerations

### See other Frequency Converting Device Measurements

## What is Harmonic Distortion?

Harmonics are multiples of any signal appearing at the mixer input and also multiples of the LO input. The distortion of the mixer's output characteristics caused by these harmonics is referred to as harmonic distortion. Harmonic distortion is caused by non-linearities in the device.

Harmonics are NOT signals created by two or more signals interacting (mixing); these signals are known as intermodulation products, which result in intermodulation distortion.

## Why Measure Harmonic Distortion?

- It can degrade the performance of devices connected to the output of the mixer.
- The harmonics can also mix with other signals present in the mixer, adding to the intermodulation distortion of the mixer.

## How to measure Harmonic Distortion

The harmonics can be measured using the PNA with Frequency Offset (option 80). The frequency of the LO to the mixer is set to zero and multiplier of the RF input is used to set the IF frequency (the harmonic). The equipment setup is shown below.

Since harmonics are specified in dBc, the fundamental RF and both the second and third harmonics are measured and the differences calculated. Multiple channels can be used to do this.

1. Connect the equipment.
2. Setup the measurement for calibration. See also Measurement and Accuracy Considerations.

Use three channels and frequency offset mode:

Channel 1 = F1 to F2

Channel 2 = F1 to 2F2 (frequency offset mode, multiplier = 1)

Channel 3 = F1 to 3F2 (frequency offset mode, multiplier = 1)

- Perform a source power calibration and receiver power calibration over the entire frequency range. See Measurement and Accuracy Considerations.

- Reduce the frequency span and increase the frequency offset multiplier on Channels 2 and 3:

Channel 2 = F1 to F2 (frequency offset mode, multiplier = 2)

Channel 3 = F1 to F2 (frequency offset mode, multiplier = 3)

**Note:** Because the frequency span has been changed from that used for calibration, the source and receiver calibrations will be interpolated.

- Connect the DUT, make the measurement, and calculate the harmonic response:

Set up markers on Channels 1, 2 and 3, and determine the difference between the marker values to get the dBc value of each harmonic.

Channel 1 - Channel 2 = 2nd harmonic (dBc)

Channel 1 - Channel 3 = 3rd harmonic (dBc)

**Note:** Be sure to set the markers to the appropriate stimulus. Channel 2 markers should be set to twice the frequency of Channel 1 markers. Channel 3 markers should be set to three times the frequency of Channel 1 markers.

---

## Measurement and Accuracy Considerations

### Equipment Setup Considerations

- A filter must be used at the input of the mixer to remove the PNA source harmonics.

### Calibrations

- If your PNA has the Frequency Converter Application (FCA), you can perform a Scalar Mixer Calibration to obtain a more accurate measurement.



## Return Loss and VSWR

---

[What are Return Loss and VSWR?](#)

[Why Measure Return Loss and VSWR?](#)

[How to Measure Return Loss and VSWR](#)

[See other Frequency Converting Device Measurements](#)

### What is Return Loss and VSWR?

Return loss and VSWR are both linear reflection measurements, even when testing frequency conversion devices, because the reflected frequency is not converted. These measurements are essentially the same as for filters and amplifiers. Learn more about [Reflection Measurements](#).


### Why Measure Return Loss and VSWR?

Devices which have poor return loss and VSWR result in loss of signal power or degradation of signal information.


### How to Measure Return Loss and VSWR

Setup the PNA measure return loss and VSWR as you would any two-port device. Connect your frequency converting device as shown in the following diagrams:


#### RETURN LOSS AND VSWR OF MIXER INPUT PORT

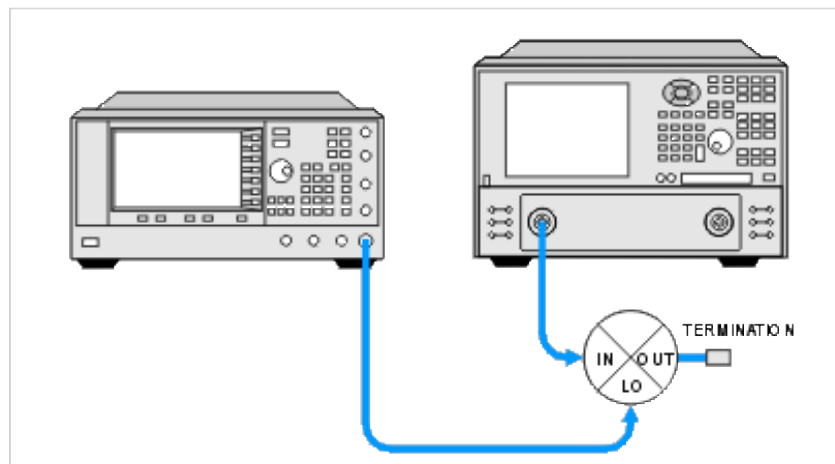

#### RETURN LOSS AND VSWR OF MIXER OUTPUT PORT

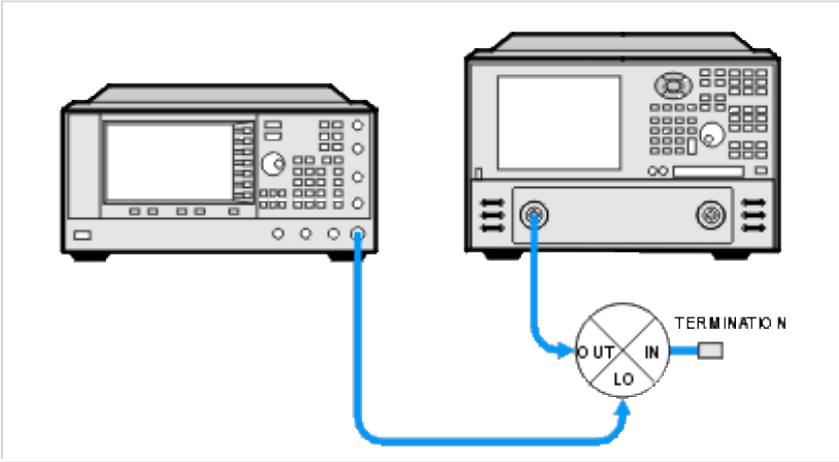

**RETURN LOSS AND VSWR OF MIXER LO PORT**

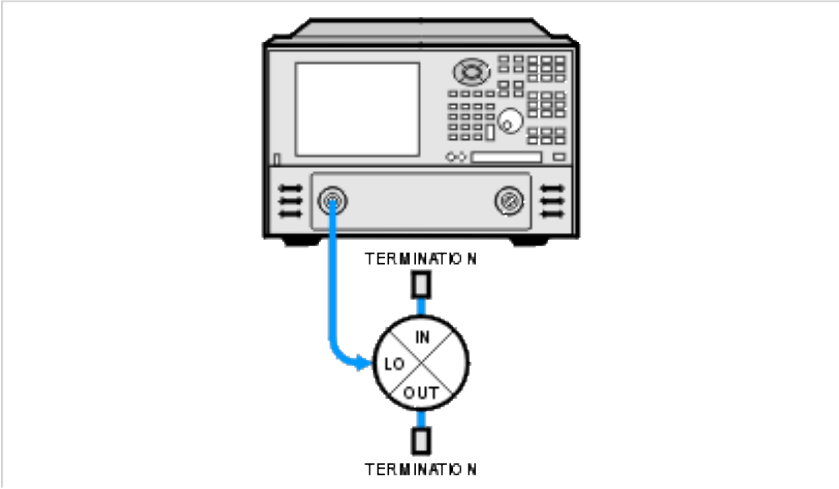

## Frequency Converter Application Known Issues

---

To see the current list of known FCA issues, please visit <http://na.tm.agilent.com/fca/> and click the known FCA issues link.

## Frequency Converter Application

---

The Frequency Converter Application ([Option 083](#)) simplifies testing of frequency converting devices. It includes the following:

- Advanced calibration techniques that provide exceptional amplitude and phase accuracy.
- Control of external signal sources for use as local oscillators.
- A graphical set-up dialog box that lets you:
  - quickly set up the PNA for single or dual conversion devices.
  - calculate and choose where mixing and image products will fall.

For more information, see the following topics:

[Using the FCA](#)

[Configure Your Mixer](#)

[FCA Calibrations](#)

[Configure an External LO Source](#)

For a detailed understanding of FCA, visit [www.Agilent.com](http://www.Agilent.com) and search for AN 1408-1, AN1408-2, and 1408-3.

**Note:** Please submit FCA issues that you find, as well as enhancement requests, to [fca\\_support@agilent.com](mailto:fca_support@agilent.com)  
See [Known Issues with the FCA](#)

---

## Using the Frequency Converter Application (Option 083)

---

### [Overview](#)

### [Create a Measurement](#)

### [FCA Measurements Offered](#)

### [FCA Measurement Settings](#)

#### [Change a Measurement](#)

#### [Speed Up Fixed Output SMC Measurements](#)

#### [Use Nominal Incident Power](#)

#### [Select X-axis Display](#)

#### [Save Trace Data](#)

#### [Avoid Spurs](#)

---

**Note:** Please submit FCA issues that you find, as well as enhancement requests, to [fca\\_support@agilent.com](mailto:fca_support@agilent.com) (See Known FCA Issues.)

---

Not sure if your analyzer is equipped with Option 083? [Here's how to identify your analyzer.](#)

### **Other Frequency Converter Application topics**

## Overview

The following is an overview of how to make an FCA measurement:

1. DECIDE to make either a Scalar measurement or Vector measurement. The calibration method is unique to each of these. [See a comparison of these two measurement types.](#)
2. CREATE and [configure](#) a default [Conversion loss](#) (SC21 or VC21) measurement: [Learn how.](#)
3. CHANGE the measurement if you want to measure something other than SC21 or VC21. Learn the various FCA [measurements that are offered](#) and how to [CHANGE](#) an FCA measurement.
4. [Setup and CALIBRATE](#) your Scalar or Vector measurement.


---

**Note:** An FCA measurement and a non-FCA measurement can NOT reside on the same channel.


---

## How to CREATE a Frequency Converter Application Measurement


Use any of the following methods to open the Choose Application Measurement dialog box:

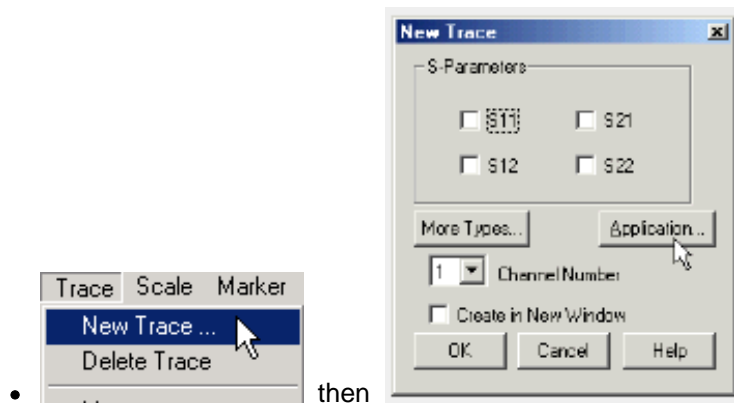

OR



Then select one of the following default conversion loss measurements:

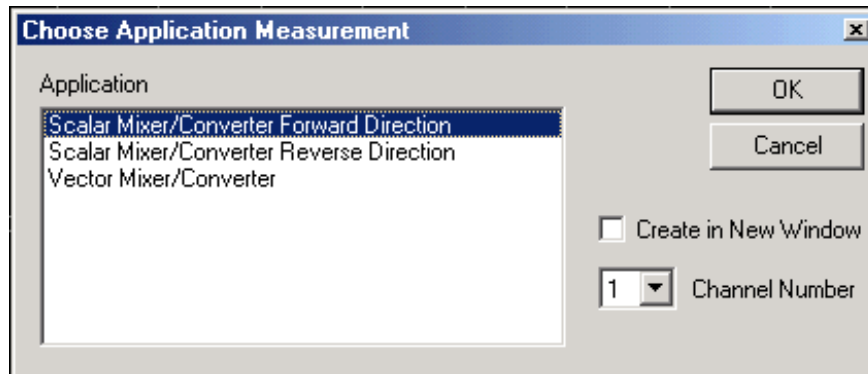

---

**Note:** Each of these three measurements must be created in a separate channel. They can NOT share the same channel.

---

Learn to make this selection using the [front panel interface](#)

### FCA Measurements Offered

Learn how to [change from the default measurement](#).

**Important Note:** Connecting your DUT to the PNA using FCA:

**RF** and **IF** terminology is NOT used in the FCA because the PNA does not know how the DUT is labeled or how it will be used. Instead, the general terms INPUT and OUTPUT are used to describe the following PNA behavior:

- INPUT - the stimulus frequencies, BEFORE conversion by your DUT.
- OUTPUT - the response frequencies, AFTER conversion (either UP or DOWN) by your DUT. Specify UP or DOWN conversion in the [Configure Mixer dialog box](#).

**Vector** (Forward Direction Only because of the use of a reference mixer)

- **VC21 Conversion Loss/Gain (default)** - stimulus at Port 1
- **S11** - stimulus at Port 1
- **S22** - stimulus at Port 2

**Scalar Mixer/Converter (Forward Direction)**

- **SC21 Conversion Loss/Gain (default)** - stimulus at Port 1
- **S11** at Input frequency - stimulus at Port 1
- **S22** at Output frequency - stimulus at Port 2
- **Incident Power** Absolute R1 power at Input frequency - stimulus at Port 1
- **Output Power** Absolute B power at Output frequency - stimulus at Port 2

**Scalar Reverse Direction**

- **SC12 Conversion Loss/Gain (default)** - stimulus at Port 2
- **S11** at Output frequency - stimulus at Port 1
- **S22** at Input frequency - - stimulus at Port 2
- **Incident Power** Absolute R2 power at Input frequency - stimulus at Port 2
- **Output Power** Absolute A power at Output frequency - stimulus at Port 1

---

**Note:** With PNA revision 4.0 you can do **FIXED OUTPUT** measurements. Learn how to [speed up your fixed output measurements](#).


---

### Understanding Scalar FORWARD and REVERSE Mixer measurements


Mixers are typically reciprocal devices ( $S_{21} = S_{12}$ ) and are therefore used and measured in both directions. The FCA allows you to make Scalar Mixer measurements in the forward and reverse directions without reconnecting your device. To help avoid confusion, the following diagrams do not use the traditional mixer labels **RF** and **IF**, but instead ports 1 and 2. The LO port is not relevant to this discussion.

**Input** is the stimulus frequencies and **Output** is the response frequencies that are used in the [Mixer setup dialog box](#).

## FORWARD

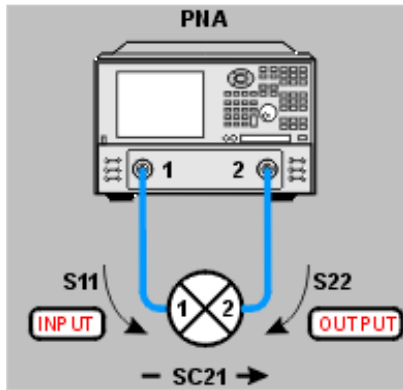

## REVERSE

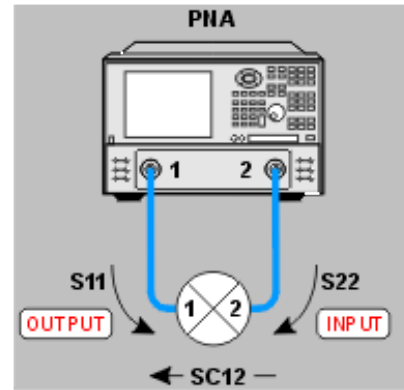

### Note:

A and R1 are port 1 receivers


B and R2 are port 2 receivers

## FCA Measurement Settings

Most of the FCA measurement settings in the remainder of this topic are made using the following menu selection. The choices will be slightly different depending on the active FCA measurement.

### How to select several FCA measurement settings

First create an FCA measurement. Then:

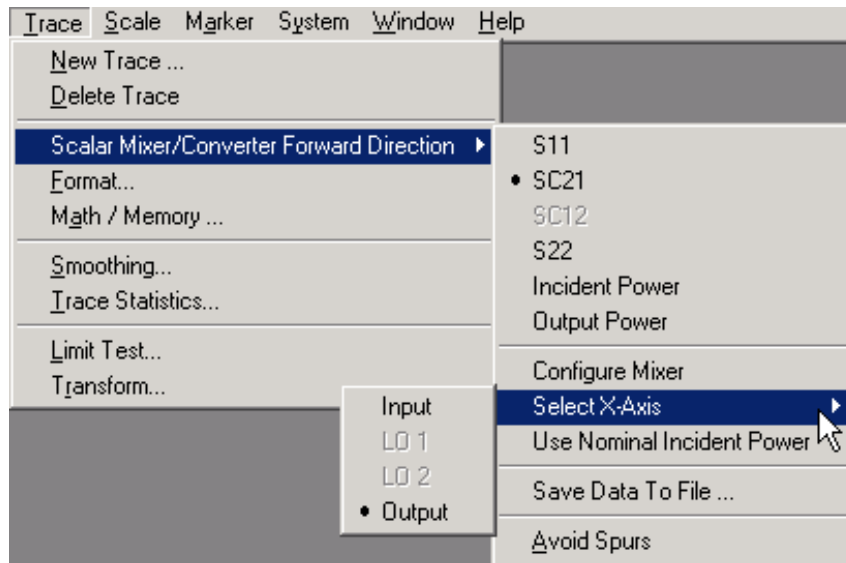

Learn to make this selection using the [front panel interface](#)

## How to CHANGE a Frequency Converter Application Measurement

Select an FCA measurement. Then:





- or use the previous **Trace** menu selection

## Speeding Up Fixed Output SMC Measurements

Fixed output SMC measurements require that an external LO source step in frequency. This can be extremely slow depending on your measurement setup. The following three feature selections together will significantly speed up your fixed output measurement:

- BNC External LO trigger method
- Cal Set Application Choice - Select **SMC Rsp**
- Use Nominal Incident Power

## Use Nominal Incident Power

Each data sweep of a fully corrected SC21 measurement actually requires THREE data sweeps. Two of the sweeps are not displayed. When you select Use Nominal Incident Power, the reference receiver (R1 or R2) does not measure incident power. Instead, the incident power is assumed to be at the level that was set with the Source Power Calibration that is done as part of every SMC measurement. The degradation in accuracy is very negligible.

This selection eliminates a sweep ONLY when either:

- Output Power is measured or
- **SMC Rsp** Cal Type is applied.

This selection applies to all SMC measurements.

See how to select Use Nominal Incident Power.

## Select X-axis Display for FCA Measurements

FCA measurements typically have more than one swept parameter. You can choose to view the response (output) of the measurement on the Y-axis while displaying any of the swept parameters (Input, LO1, LO2, Output) on the X-axis of the PNA display.


For example, the following image shows an SMC Forward Fixed Output response versus the swept Input.

Output: 100 MHz (data trace)

Input: 2 GHz to 23 GHz (X-axis)

LO: 1.9 GHz to 22.9 GHz (not shown)

Marker annotation shows Output power at Input frequency.

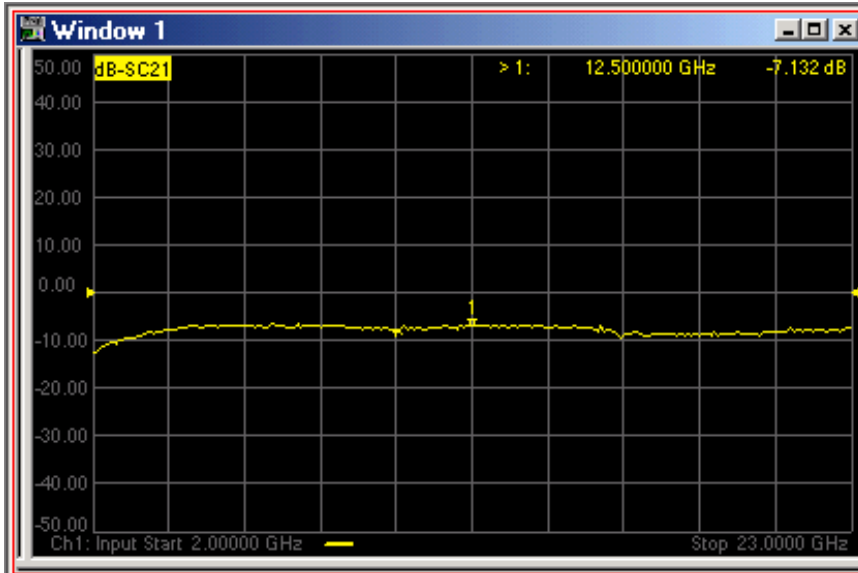


[See How to Select X-axis Display](#)

## Save Trace Data

You can save your Frequency Converter measurement data in S2P format to disk.

**Note:** This is the only method to save Frequency Converter .S2P files. Do NOT click **File, Save As...** to save these S2P data files.

[See How to Save Trace Data](#)

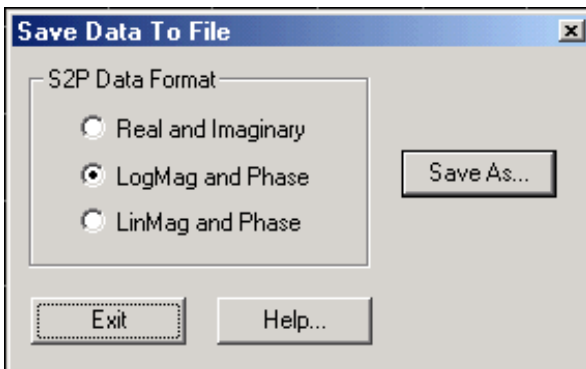

## Save Data to File dialog box help

Allows you to save Frequency Converter measurement data to an S2P file. The data is saved in S2P format much like standard PNA data. [Learn more about .S2P files.](#)

**Note:** This is the only method to save Frequency Converter .S2P files. Do NOT click **File, Save As...** to save these S2P data files.

**S2P Data Format** Select the data format. This selection is independent of the PNA display.

**Save As** Click to specify a file name and location for the saved data.

**Exit** Closes the dialog box without saving the data. To save the data, you must click on the Save As button before clicking the Exit button.

### Notes:

Each record contains 1 stimulus value and 4 parameters (total of 9 values) as follows:

Stim Real(p1) Imag(p1) Real(p2) Imag(p2) Real(p3) Imag(p3) Real(p4) Imag(p4)

where **pX** is the parameter depending on measurement type:

| Measurement Type       | p1          | p2           | p3                  | p4  |
|------------------------|-------------|--------------|---------------------|-----|
| Scalar                 | S11         | SC21 (FWD)   | SC12 (REV)          | S22 |
| Vector                 | S11         | VC21         | VC12                | S22 |
| Mixer Characterization | Directivity | Source Match | Reflection Tracking | M21 |

- If correction is OFF, data is only saved for the active parameter. Zeros are saved for all other parameters.
- If correction is ON, data is saved for all of the parameters.

All files contain the following Header Information: Brackets [ ] contain parameters.

```
!Agilent [Instrument Model Number]: [version]
!Mixer S2P File: [Mixer Measurement Type]
!Parameters: [Parameter List]
!Calibration State: [On/Off]
```

```
!# Begin Mixer Setup
![Mixer Setup parameters listed here]
![Mixer Parameter 1]
.
.
![Mixer Parameter n]
!# End Mixer Setup

[S2P data here]
```

## Avoid Spurs

The Avoid Spurs feature of the Frequency Converter Application attempts to prevent unwanted mixing products from appearing on the PNA screen. The Avoid Spurs feature does not significantly impact measurement speed.

---

**Note:** The Avoid Spurs feature is OFF by default for FCA calibrations. For highest accuracy, make measurements with the Avoid Spurs feature at the same state (ON or OFF) as was used when calibrating.

---

See [how to Avoid Spurs](#) OR Check **Avoid Spurs** on the [Mixer Setup](#) dialog box.

### **Description**

A spur, or spurious signal, is a term used to describe the unwanted product of two signals mixing together. When you configure the mixer setup dialog box for a desired Output, the PNA computes the frequencies of potential unwanted signals. By manipulating internal PNA hardware, these signals are avoided and do not appear on the PNA display. This means you do not need to use external filters to prevent spurious signals from appearing on the PNA display.

The time required for the PNA to compute the frequencies of unwanted spurious signals MAY be noticeable depending on the number of data points in your measurement. However, once computed, the time required for the PNA to avoid the spurs is usually insignificant.

### **Limitations**

The Avoid Spurs utility cannot avoid every spur. However, when there is a choice of spurs to avoid, it will avoid the largest spur.

### **The Computation of Avoided Spurs**

The Avoid Spur computer avoids the following spurs:

- LO, and its interaction with internal PNA components, and 16 of its harmonics.
- Input frequencies and 16 of its harmonics.
- Undesired Image frequencies (Sum or Difference) and 16 of its harmonics.

## Frequency Converter Application (Option 083) Calibrations

---

Frequency Converter Application (Option 083) offers two advanced calibration choices for mixer or converter measurements that provide exceptional amplitude and phase accuracy.

### [Comparison of Scalar and Vector Mixer Cals](#)

#### [SMC Setup and Overview](#)

#### [VMC Setup and Overview](#)

#### [FCA Calibration Process Diagram](#)

#### [How to Perform an FCA Calibration](#)

#### [Apply an FCA Cal Set](#)


Not sure if your analyzer is equipped with Option 083? [Here's how to identify your analyzer.](#)

To learn more, see [www.Agilent.com](http://www.Agilent.com) and search for "Mixer Transmission Measurements Using The Frequency Converter Application (AN 1408-1)"

Please submit FCA issues that you find, as well as enhancement requests, to [fca\\_support@agilent.com](mailto:fca_support@agilent.com) (See [Known FCA Issues.](#))

### [Other Frequency Converter Application topics](#)


## Comparison of Scalar and Vector Mixer Cals

|                                                                                                     | Scalar Mixer Calibration                                                                                                                                                                                 | Vector Mixer Calibration                                                                                                                                                                                                                                                                                                                                                                              |
|-----------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  <b>Overview</b> | <p>Provides highest Scalar (amplitude only) accuracy for measurements of conversion loss/gain.</p> <p>Combines SOLT and power-meter calibration.</p> <p>Simpler setup than Vector Mixer Calibration.</p> | <p>Provides unparalleled accuracy for measurements of relative phase and absolute group delay.</p> <p>Uses combination of SOLT standards and a reciprocal mixer/filter pair during calibration.</p> <p>More complicated setup and calibration procedure than Scalar Mixer Calibration.</p> <p>After calibration, both reciprocal and non-reciprocal mixers and converters can easily be measured.</p> |
| <b>Types of Transmission Measurements</b>                                                           | Can test in both forward (SC <sub>21</sub> ) and reverse (SC <sub>12</sub> ) directions.                                                                                                                 | <p>Amplitude response VC<sub>21</sub></p> <p>Phase response</p> <p>Group delay</p>                                                                                                                                                                                                                                                                                                                    |

|                                       |                                                                                               |                                                                                               |
|---------------------------------------|-----------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------|
| <b>Options and Equipment Required</b> | Option 014                                                                                    | Option 014                                                                                    |
|                                       | Option 080                                                                                    | Option 080                                                                                    |
|                                       | Option 083                                                                                    | Option 081                                                                                    |
|                                       | Mechanical cal kit or ECal module                                                             | Option 083                                                                                    |
|                                       | Power meter and sensor                                                                        | Mechanical cal kit or ECal module                                                             |
|                                       | Agilent 82357A USB/GPIB Interface (included with Frequency Converter Application, Option 083) | Calibration mixer/filter combination (must be reciprocal $S_{21} = S_{12}$ .)                 |
|                                       |                                                                                               | Reference mixer/filter combination                                                            |
|                                       |                                                                                               | External source                                                                               |
|                                       |                                                                                               | Agilent 82357A USB/GPIB Interface (included with Frequency Converter Application, Option 083) |

Note: Find more information comparing these two mixer calibration types at <http://www.tm.agilent.com>. Click "Library" and use the search function to find the white-paper titled "Comparison of Mixer Characterization Using New Vector Characterization Techniques".

### SMC Calibration Setup

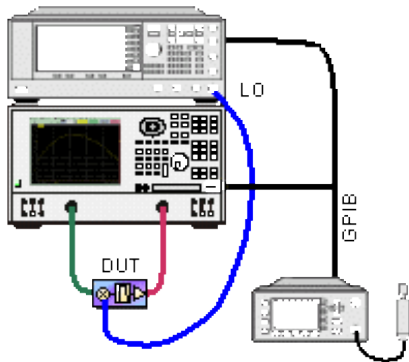

Connect external source and power meter to the PNA GPIB using either:

- The Agilent 82357A USB/GPIB Interface - **highly recommended** - allows for the use of a remote PC to control the PNA.
- The standard GPIB Interface - with the following limitations:
  - The PNA cannot be controlled remotely as talker / listener over GPIB. First put the PNA in System Controller mode. Learn how.
  - Available only on PNA releases 4.2 and later.

Learn about supported power meters and sensors.


Learn how to Configure an External LO Source

### Overview of the Scalar Mixer Calibration

The Calibration Wizard guides you through this process.

1. Perform two 2-port calibrations: one over the INPUT frequencies and one over the OUTPUT frequencies of the DUT. (If your DUT is a linear device, the calibration uses only the INPUT frequency range.) Use either a mechanical calibration kit or an ECal module.
2. Connect a power meter sensor to PNA Port 1. At each step of the input and output frequency, the PNA measures:
  - input match of the power sensor
  - source power of the PNA

## VMC Calibration Setup

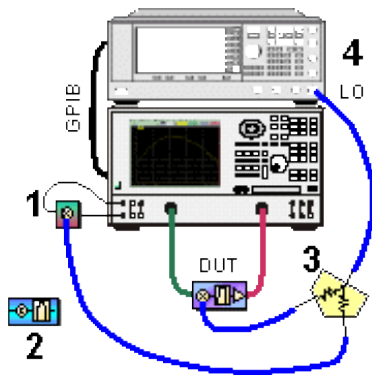

1. **Reference mixer** whose signal is synchronously converted with the device under test. This means the reference mixer and the mixer or converter-under-test use LO signals in a constant frequency and phase relationship.

- Connect the Reference Mixer INPUT to PNA **Ref 1 Source out**
- Connect the Reference Mixer OUTPUT to PNA **Rcvr R1 In**

2. **Calibration mixer/filter** combination that meets the following requirements:

- The mixer must be reciprocal. This means that it has the same magnitude and phase response in the up-converting and down-converting directions ( $C_{21} = C_{12}$ ).
- If the Input and Output frequency ranges are overlapping, the mixer must have Input to Output Isolation greater than 10 dB more than the conversion loss in the overlapping range.
- The filter must reject the undesired mixing product at the output of the cal mixer. For example, if you have selected the **Input + LO** mixing product in the cal mixer setup, you must use a high-frequency bandpass filter to reject the **Input - LO** mixing product when characterizing the cal mixer. If this is not practical, see further details at [www.Agilent.com](http://www.Agilent.com) and search for "Mixer Transmission Measurements Using The Frequency Converter Application (AN 1408-1)".

3. **Power splitter**

4. **LO Source(s)** Connect external sources to the PNA GPIB using either:

- The Agilent 82357A USB/GPIB Interface - **highly recommended** - allows for the use of a remote PC to control the PNA.
- The standard GPIB Interface - with the following limitations:

- The PNA cannot be controlled remotely as talker / listener over GPIB. First put the PNA in System Controller mode. [Learn how.](#)
- Available only on PNA releases 4.2 and later.

Learn how to [Configure an External LO Source](#)

### **Overview of the Vector Mixer Calibration**


The Calibration Wizard guides you through this process. The first three steps characterize the calibration mixer that is used as the THRU standard during the calibration process.

1. Perform two [2-port calibrations](#) over the INPUT and OUTPUT frequency ranges of the DUT. Use either a mechanical calibration kit or an ECal module.
2. Characterize the input and output match of the [calibration mixer/filter combination](#) with the external LO connected and the output terminated with an open, short, and load.
3. Connect a reference mixer/filter combination between the Source Out and Rcvr R1 front-panel connectors. Connect the output port of the calibration mixer/filter combination to PNA Port 2 (or at the end of the cable attached to the port).
4. With the PNA in frequency offset mode, measure the calibration mixer/filter combination as the THRU calibration standard.
5. The PNA calculates the error terms necessary to make corrected phase measurements of your mixer/converter under test.

### **The FCA Calibration Process**

Click a box to learn about that step.




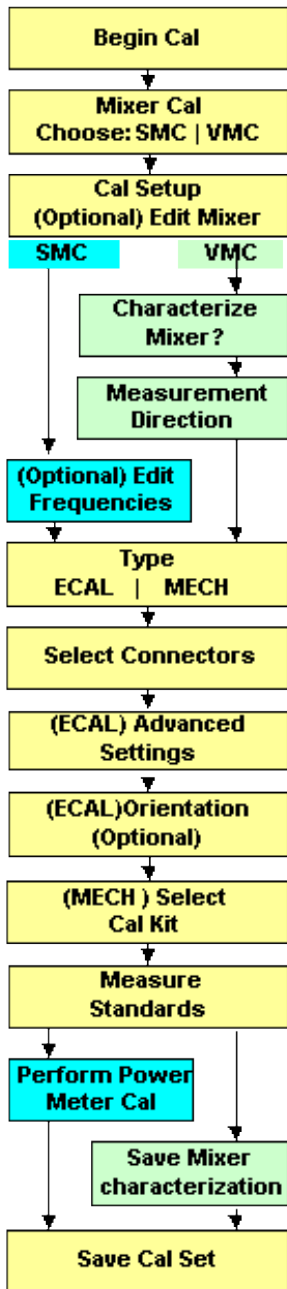


**Note:** In the above diagram and following procedure, the color coding indicates that the step is performed either in **SMC ONLY** or **VMC ONLY**. The **yellow** blocks indicate the steps that are common to both calibration methods.

## How to Perform an FCA Calibration

Begin an FCA calibration as you would any PNA calibration:

1. Click **Calibration**, then **Calibration Wizard**.
2. Then select **Mixer Calibrations**.

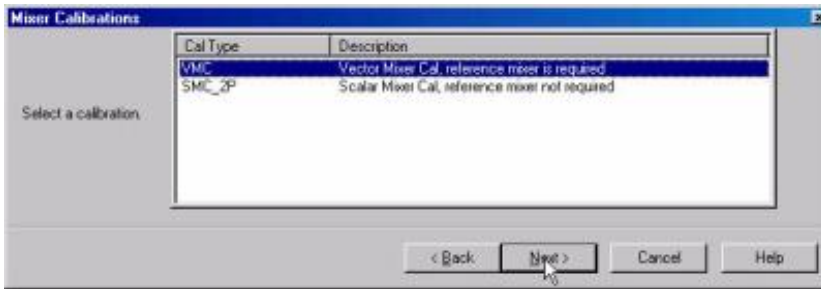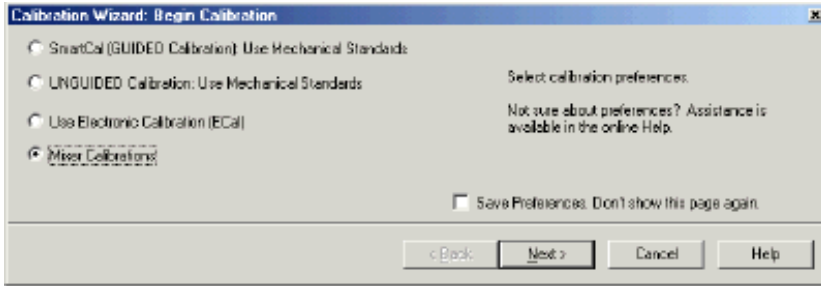


**Mixer Calibrations** dialog box help  
See this step in the FCA cal process

Allows you to select a mixer/converter calibration method:

**VMC Vector Mixer Cal** Selects the Vector Mixer Cal.

**SMC\_2P Scalar Mixer Cal** Selects the Scalar Mixer Cal.

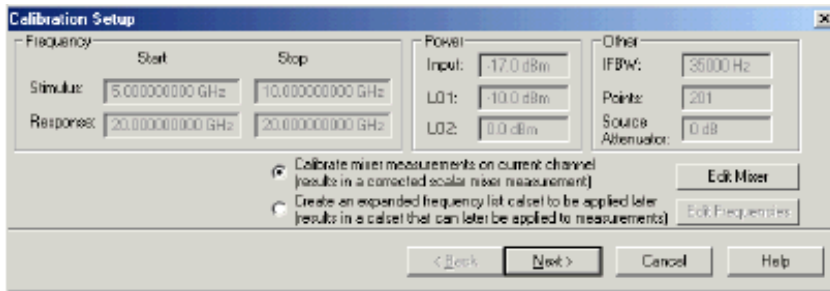

## Calibration Setup dialog box help

Allows you to review and change the settings for your FCA calibration.

- To change **Frequency** and **Power** settings click **Edit Mixer**
- To change **Other** settings (IFBW, Points, Attenuator) scroll or type in a new value.

**Edit Mixer** Displays the [Configure Mixer](#) dialog box.

### SMC ONLY

#### **Calibrate mixer measurements on current channel (results in a corrected scalar mixer measurement).**

Allows you to make corrected scalar measurements of your DUT on the current channel. When the calibration is completed, a Cal Set is saved and the PNA automatically creates an SC<sub>21</sub> measurement.

#### **Create an expanded frequency list calset to be applied later (results in a calset that can later be applied to measurements).**

Allows you to select a calibration frequency range that is wider than the frequency range of your DUT. When the calibration is completed, a Cal Set is saved but the PNA does NOT automatically create a measurement. To make a measurement, you must [apply the Cal Set](#) to the desired channel and select a measurement.

**Edit Frequencies** Enabled when **Create an expanded...** is selected. Displays the [Frequencies dialog box](#) where you can expand the frequency range of the calibration beyond the range of your DUT. [Learn more.](#)

### VMC ONLY



## Select Calibration Procedure dialog box help

Allows you to perform calibration mixer characterization only or perform a full system calibration.

### What is Calibration Mixer Characterization?

For a brief explanation, see [Calibration Mixer](#) (Step 2).

For a detailed explanation, see [www.Agilent.com](http://www.Agilent.com) and search for "Mixer Transmission Measurements Using The Frequency Converter Application (AN 1408-1)"

### Procedure

**Calibration Mixer Characterization Only** Performs a 2-port calibration and characterizes the calibration mixer. Does not require a reference mixer. Choose this if you want to save the mixer characterization data to a file that will be downloaded later as part of a full system calibration.


**Full System Calibration** Performs a full system calibration. Requires a reference mixer.

**Characterization** - Only available if performing a Full System Calibration

**Perform calibration mixer characterization** Characterizes the calibration mixer. Choose this selection if you do NOT have the mixer characterization data on file.

**Load characterization from file** Loads calibration mixer characterization data from your file. Use the **Browse** function to locate the file.

## VMC ONLY

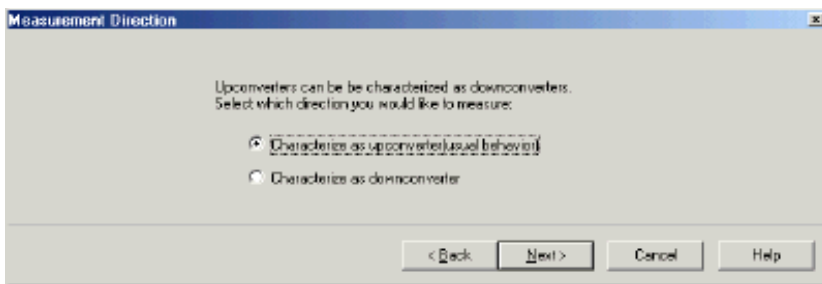

## Measurement Direction dialog box help

This dialog box appears ONLY if your settings in the [Mixer Setup](#) dialog box indicate that your DUT is being tested as an upconverter (input < output). It allows you to characterize the [Calibration Mixer](#) as a downconverter (input > output) or an upconverter.

**Characterize as upconverter (usual behavior)** The disadvantage of characterizing as an upconverter is that you must use an expensive high-frequency filter at the output of the calibration mixer.

**Characterize as downconverter** Characterizes the calibration mixer as a downconverter which allows you to use a more economical low-frequency filter.

## Expanded SMC Calibration

An SMC calibration does not require that the calibration input and output frequencies match the current mixer IF frequency calculations.


**For example**, you can perform an SMC calibration over the following frequencies:

- Input frequency range: 10 MHz to 20 GHz
- Output frequency range: 10 MHz to 20 GHz.

Once this calibration is performed, you can save and apply it to any SMC measurement with Input and Output frequencies between 10 MHz and 20 GHz that share the same physical measurement setup. Learn how to [apply an SMC calibration](#).

To perform an expanded SMC calibration, in the [Calibration Setup](#) dialog box, select **Create an expanded frequency list calset to be applied later**.

For high measurement accuracy, use a high number of data points. Learn more about [Interpolation Accuracy](#).

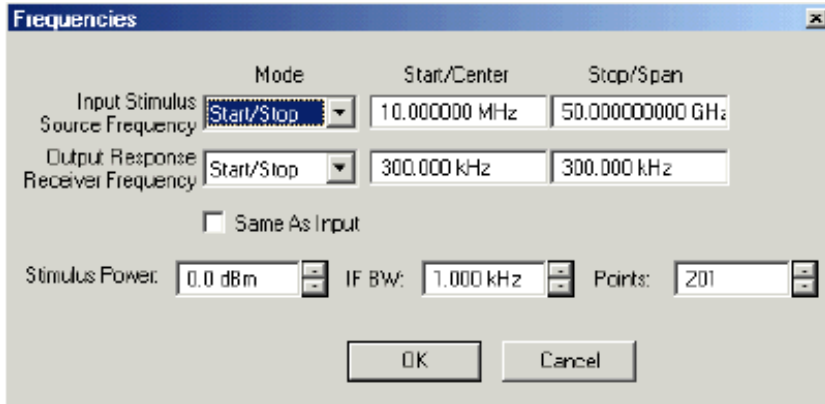

### Frequencies dialog box help


Allows you to edit your calibration frequency range so that it is wider than the frequency range of your DUT. [Learn more...](#)

**Mode** Selects the format to specify the frequency information in your test setup. Frequency information can be specified using start/stop or center/span formats.

**Start/Center** Allows you to enter the start frequency (for Start/Stop mode) or the center frequency (for Center/Span mode).

**Stop/Span** Allows you to enter the stop frequency (for Start/Stop mode) or the frequency span (for Center/Span mode).

**Same As Input** Select this checkbox to set the output response frequency the same as the input stimulus frequency.

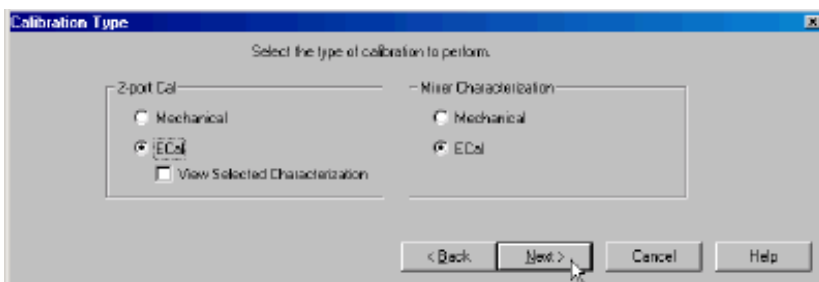

## Calibration Type dialog box help

Allows you to specify either ECal or mechanical calibration.

2-port Cal

**Mechanical** Specifies mechanical calibration.

**ECal** Specifies ECal calibration.

**View Selected Characterization** Check to invoke a dialog box to [View the Selected Characterization](#) (user or factory) for performing the ECAL. Learn more about [ECal User Characterization](#).

If the frequency range of the active channel is greater than that of the selected characterization, a **Caution: Additional Standards Required** message is displayed. To correct the problem, perform one of the following solutions:

- Reduce the frequency range of the active channel.
- Select a different characterization that covers the required frequency range.
- Re-characterize the module with an increased frequency range.

### VMC ONLY:

Mixer Characterization

**Mechanical** Specifies mechanical calibration.

**ECal** Specifies ECal calibration.

Learn more about [Mixer Characterization](#)


### If using ECal:

In the [Advanced Settings dialog box](#), choose the settings for your ECal calibration.

If Adapter Removal calibration was selected, the [Select DUT Connectors dialog box](#) is displayed. Select the connectors for port 1 and port 2.

In the [Electronic Calibration Steps dialog box](#), follow the instructions for using the ECal module.

### If using Mechanical Cal Kit

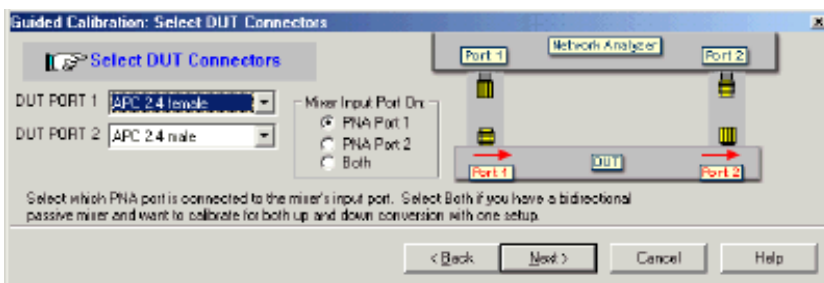

## Select DUT Connectors dialog box help

Allows you to specify the connector type of each DUT port.

**DUT Port 1** Specify the connector type of DUT port 1.

**DUT Port 2** Specify the connector type of DUT port 2.

**Note:** If your DUT connectors are:

- **Waveguide** Change the system impedance to 1 ohm before performing a calibration. See [Setting System Impedance](#).
- **Not listed** (male and female) Select **Type A** as the connector type. Type A requires a calibration kit file containing the electrical properties of the standards used for calibration (see [Calibration kits](#)).
- **Unspecified** (like a packaged device) Select **Type B** as the connector type. Type B requires a calibration kit file containing the electrical properties of the standards used for calibration (see [Calibration kits](#)).
- **Non-insertable** Guided Cal automatically performs an [Adapter Removal](#) calibration. This requires that you have an adapter that has the same connectors as the DUT.

### SMC ONLY:

**PNA Port 1** Make this selection to calibrate for ONLY forward direction measurements. Input frequencies are associated with the DUT port that is connected to PNA port 1.

**PNA Port 2** Make this selection to calibrate for ONLY Reverse direction measurements. Input frequencies are associated with the DUT port that is connected to PNA port 2.

**Both** Provides Scalar calibration for both Forward and Reverse SMC measurements. Two cal sets are saved. You apply the appropriate calibration to the measurement. [Learn more about SMC Forward and Reverse measurements](#).



### Select Cal Kits dialog box help

Allows you to select the calibration kit used with each measurement port. The list for each port displays kits having the same connector type as the DUT.

**PORT 1** Lists the calibration kits available with port 1

**PORT 2** Lists the calibration kits available with port 2

**Insertable** Select if your DUT is an insertable device.

**Adapter Removal** Select if your DUT is a noninsertable device and you want to perform an Adapter Removal calibration.

**Unknown Thru** Select if your DUT is a noninsertable device and you want to perform an Unknown Thru calibration.



### Measure Calibration Standards dialog box help

Illustrates how to connect the calibration standard specified in the prompt. The illustration will vary depending on which calibration standard you are measuring. The illustration will also vary if:

- you are using an ECal module
- you are performing a calibration-mixer characterization or a full system calibration
- your test setup includes a single LO or a dual LO
- you selected "Characterize as downconverter" in the Measurement Direction dialog box. In this case, the illustration shows the mixer configured backwards for reflection measurements. The mixer's output is connected to the PNA's test port 2, and the calibration standard (or ECal module) is connected to the mixer's input.

**Measure & Next** Measures the mechanical standard and continue to the next calibration step.

**Back** Returns to the previous dialog box.


**Next** Appears only after clicking Back. Allows you to proceed to the next required step. Does NOT make a measurement.

**ReMeasure** Appears only after clicking Back. Allows you to remeasure a standard.

### SMC ONLY

**For both ECal and Mechanical calibration:**



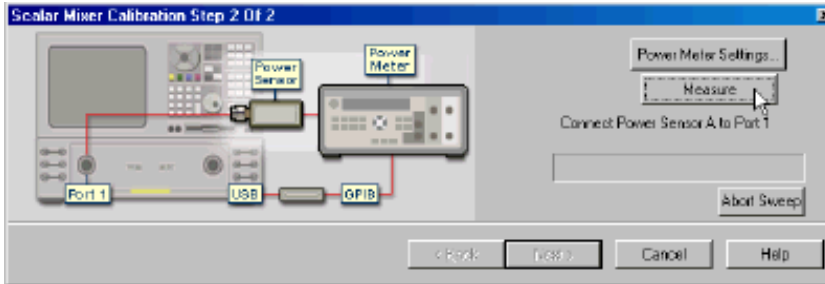

### Scalar Mixer Calibration Power Cal dialog box help.

Prompts you to perform the power-meter section of the calibration.

**Note:** SMC calibration performs 10 averages at the beginning and at the end of the power cal step to ratio the difference between normal and offset R1 measurements in the calibration band of frequencies. The averaging is done to remove a reasonable amount of noise from the ratio measurement.

- Connect your power sensor to the port shown in the diagram. The diagram will vary depending if port 1 was designated as "output" "input" or "both" in the [Select DUT Connectors dialog box](#).
- Begins the power meter calibration on Port 1, 2, or both.

**Power Meter Settings** Invokes the [Power Meter Settings](#) dialog box. [Learn about Equipment setup.](#)


**Note:** From Power Meter Settings, you can use the [Power Loss Compensation Table](#) to compensate for an adapter used to connect the power meter sensor.

**Measure** Begins the power meter measurements and then continues to the next step.

**Back** Returns to the previous dialog box.

**Next** Continues to the next calibration step. Does NOT make a measurement.

### VMC ONLY

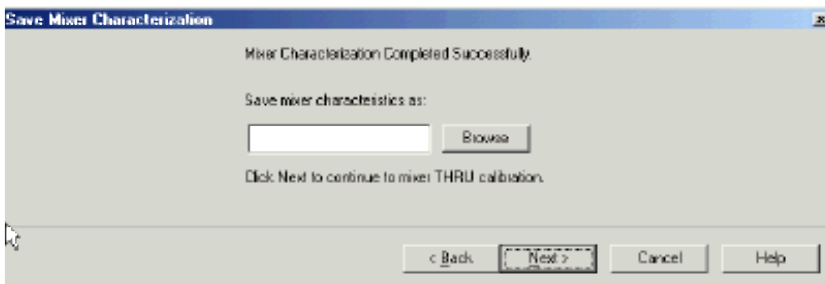

### Save Mixer Characterization dialog box help

Allows you to save the characterization data of your [calibration mixer](#).

**Browse** Navigate to the location where you want to save the characterization data of your calibration mixer. Either use the default file name or enter a custom file name.

**Next** Saves the mixer characterization file and continues with the next step in the full system calibration routine.

**Finish** Replaces **Next** if you are only characterizing the calibration mixer instead of performing a full system calibration. Saves the mixer characterization file and exits the mixer characterization routine.

### Save Calibration

### If performing a full system calibration:

In the [Calibration Completed dialog box](#), click **No. Finish now** to exit the Calibration Wizard.

### Create and Apply an FCA Cal Set

You can create an FCA measurement and apply an existing Cal Set as you can with any PNA measurement. Learn about [Cal Sets](#).

When you apply an FCA Cal Set, be sure to apply the appropriate Cal Type (see table below) to the FCA measurement. The following two notes highlight subtle differences for applying SMC Cal Sets. VMC calibrations are only performed in the forward direction.

- SMC Cals save separate Cal Sets for the Forward and Reverse directions. An SMC Forward Cal Set cannot be applied to an SMC Reverse measurement and vice versa. Learn more about [Forward and Reverse Scalar measurements](#).
- A single SMC Cal Set can contain the following SMC Cal Types, allowing you to optimize Fixed Output measurements for speed versus accuracy. Learn other ways to [speed up your fixed output measurements](#).

| FCA Cal Type                                                                                | FCA Measurement |
|---------------------------------------------------------------------------------------------|-----------------|
| <b>SMC_2P:</b> (Response + Input + Output) Most accurate                                    | SC21            |
| <b>SMC Rsp:</b> no Input or Output match - Fastest for fixed output, but not most accurate. | SC12            |
| <b>SMC Rsp + In:</b> no Output match - Best combined accuracy and speed for fixed Output.   | S11             |
| <b>SMC Rsp + Out:</b> no Input match                                                        | S22             |
|                                                                                             | Incident Power  |
|                                                                                             | Output Power    |
| <b>VMC</b> (source is Port 1)                                                               | VC21            |
|                                                                                             | S11             |
|                                                                                             | S22             |

## Configure a Mixer

---

[How to Start the Mixer Setup dialog box](#)

[Learning the Mixer Setup Dialog Box](#)

[Rules for Configuring a Mixer](#)

[Using Power Sweep for Testing Mixers](#)

[Input > LO Example](#)

[Configure Fixed Output Measurements](#)

[Fractional Multiplier Examples](#)

---

**Note:** Please submit FCA issues that you find, as well as enhancement requests, to [fca\\_support@agilent.com](mailto:fca_support@agilent.com)  
(See Known FCA Issues.)


---

### Other Frequency Converter Application topics

#### How to start the Mixer Setup dialog box

Choose any of the following methods:

[Create an FCA measurement.](#) Then

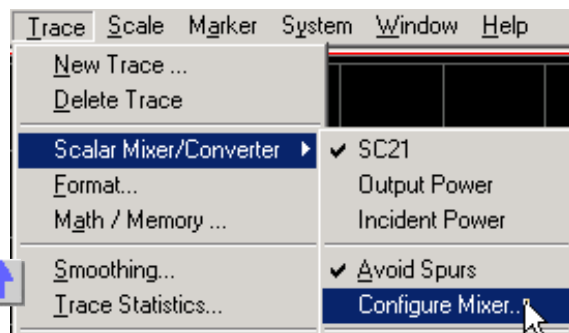

OR

[Create an FCA measurement.](#) Then press one of these buttons:



OR

[Create an FCA measurement.](#) Then

1. Click **Calibration**, then **Calibration Wizard**
2. Click **Mixer Calibration**

### 3. Click **Edit Mixer**

Learn more about using the [front panel interface](#)

## Learning the Mixer Setup dialog box

Click on sections of the image to learn about a setting.

The screenshot shows the Mixer Setup dialog box with the following settings:

| Section | Power       | Frequency Range                    | Other Settings                                                    |
|---------|-------------|------------------------------------|-------------------------------------------------------------------|
| Input   | -17.000 dBm | 1.000000000 GHz to 4.000000000 GHz | Start/Stop dropdown, Calculate IF1 & Output button                |
| LO1     | -10.000 dBm | 500.000000 MHz                     | Fixed dropdown, Input > LO checkbox, Calculate Input & Out button |
| IF1     |             | 1.500000000 GHz to 4.500000000 GHz | Start/Stop dropdown, +/- dropdown, Calculate Input & Out button   |
| LO2     | -10.000 dBm | 500.000000 MHz                     | Fixed dropdown, IF1 > LO2 checkbox, Calculate Input & IF1 button  |
| Output  |             | 2.000000000 GHz to 5.000000000 GHz | Start/Stop dropdown, +/- dropdown, Calculate Input & IF1 button   |

Buttons at the bottom: Hide Diagrams, LOs: 1 (selected), Avoid Spurs, Load..., Save..., **Apply** (highlighted), OK, Cancel, Help.

The block diagram below shows the mixer circuit with the following parameters:

- Input:** Start: 1.000000000 GHz, Stop: 4.000000000 GHz, Power: -17.000 dBm
- LO1:** Start: 500.000000 MHz, Stop: 500.000000 MHz, Power: -10.000 dBm
- IF1:** Start: 1.500000000 GHz, Stop: 4.500000000 GHz
- LO2:** Start: 500.000000 MHz, Stop: 500.000000 MHz, Power: -10.000 dBm
- Output:** Start: 2.000000000 GHz, Stop: 5.000000000 GHz

**Note:** This image shows two LOs.

**Important Note:** Connecting your DUT to the PNA using FCA:

**RF** and **IF** terminology is NOT used in the FCA because the PNA does not know how the DUT is labeled or how it will be used. Instead, the general terms **INPUT** and **OUTPUT** are used to describe the following PNA behavior:

- **INPUT** - the stimulus frequencies, BEFORE conversion by your DUT.
- **OUTPUT** - the response frequencies, AFTER conversion (either UP or DOWN) by your DUT. Specify UP or DOWN conversion using the + or - symbol for each output.

See [Fractional Multiplier Examples](#) (below)

### Mixer Setup dialog box help

Throughout the dialog box, the Mixer / converter ports are color coded (Input, LO1, IF1, LO2, Output)

## Rules for Configuring a Mixer

Red **Apply** and **OK** buttons indicate that one or more of the following settings are invalid.

1. The INPUT start frequency can NOT exceed the stop frequency.(The OUTPUT start frequency CAN exceed the stop frequency.)
2. INPUT or OUTPUT frequencies cannot be outside the range of the PNA.
3. Fixed INPUT / SWEPT OUTPUT measurements are NOT allowed.
4. Any combination of INPUT and LO which results in an OUTPUT that sweeps through zero Hz is NOT allowed.
5. The range for the numerator and denominator of a fractional multiplier is from +1 to +10. Negative values are NOT allowed.

**Power** Sets the power level of the input signal, and both LO signals.

**Frequency Format** Selects the format to specify the frequency information for each signal in your test setup. The Input, LO1, LO2, IF, and Output frequency information can be specified using start/stop or center/span formats. Only LO1, LO2, IF, and Output formats can be set to Fixed. When you select a swept LO, you can also select the information you want to display on the X-axis.

**Source Configuration Buttons** Performs the same function as the configuration buttons on the lower diagram. The current source is displayed on the button label.

**Resulting Frequencies** Either sets or calculates the frequency values for each of the signals in your test setup. For example, if you enter the Input frequency range and press the Calculate button adjacent to the Input, the PNA will calculate and display the Output frequencies.

Go to the **Mixer Setup** image


### Input > LO

These check boxes remove ambiguity when using the Calculate button to determine the INPUT frequency.

|                                                |                                                                                                                               |
|------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------|
| <input checked="" type="checkbox"/> Input > LO | Check if the <b>INPUT</b> is <b>GREATER THAN</b> the <b>LO</b><br>Clear if the <b>INPUT</b> is <b>LESS THAN</b> the <b>LO</b> |
| <input checked="" type="checkbox"/> IF1 > LO2  | Check if the <b>IF1</b> is <b>GREATER THAN</b> the <b>LO2</b><br>Clear if the <b>IF1</b> is <b>LESS THAN</b> the <b>LO2</b>   |

These boxes are only used when all 3 of the following conditions are TRUE:  
(If ALL 3 are NOT true, the PNA does not read these boxes).



1. Difference (Low) sideband  is selected for the corresponding Calculate button AND
2. Output frequency is less than the LO frequency AND
3. The Green or Blue Calculate button is used to calculate the Input frequency.

To learn more, see this example.

### Fractional Multiplier

The combination of (numerator / denominator) forms a fractional value that is multiplied by the input and LO frequency ranges (also the IF and LO2 frequency ranges for a test setup with two LOs). These values are used to Calculate the response frequency of the PNA receiver. Use the fractional multipliers to:

- replicate the action of harmonic mixers
- replicate the action of multipliers and dividers that may exist in your test setup
- tune the PNA receiver frequency to a harmonic of the mixer/converter

See [Fractional Multiplier examples](#).

[Go to the Mixer Setup image](#)

**Mixer-Product Selector** Determines whether the receivers will tune to the Sum (+) or the Difference (-) of the Input and LO frequencies. Click the adjacent Calculate button after your selection.

**Calculate buttons** Calculates frequency information based on your other mixer settings. The mixer port settings next to the Calculate button you press remain fixed. For example, in a 1-LO scenario, specify the Input and LO frequencies, specify + (sum), then click the **Calculate** button next to the Input. The input remains fixed and the output frequency range is calculated for you.

**Hide / Show Diagrams** Hides and displays the test setup diagram. Your measurement trace is displayed when the diagram is hidden.

**LOs** Click 1 or 2 to select the number of external LO sources in your test setup. When you select 2 LOs, the IF1 frequencies are set for you. Measurements of a DUT with an embedded LO are not supported at this time.

**Avoid Spurs** Check to invoke the [Avoid Spurs](#) feature.

**Load** Loads a previously-configured mixer attributes file (.mxr).

---

**Note:** A .mxr file includes an LO source name. However, It does NOT include the LO Source configuration. Therefore, when using a .mxr file that was created on a different PNA, the PNA will display an error if does not find the LO Source configuration using EXACTLY the same LO source name.

---

**Save** Saves the settings for your mixer/converter test setup to a mixer attributes file (.mxr).

**Apply** Applies the settings for your mixer/converter test setup to the measurement. The mixer setup dialog box remains OPEN. If shaded red, [see rules](#).

**OK** Applies the settings for your mixer/converter test setup to the measurement. The mixer setup dialog box CLOSES. If shaded red, [see rules](#).

**Cancel** Closes the mixer setup dialog box and does NOT apply the settings.

**Frequency Diagram:** Provides a display of the frequency information for the signals in the test setup.

**Configure Source** Displays the [External Source Configuration dialog box](#).

[Go to the Mixer Setup image](#)

## Using Power Sweep for Testing Mixers

To measure the gain compression of a mixer, you need to sweep the input power to the mixer. The input and output frequencies are fixed but offset from one another. To set Power Sweep and the input and output frequencies of the mixer under test:

1. On the mixer dialog box, set the LO frequency, identical input start and stop frequencies, and identical output start and stop frequencies. These selections create fixed input and output frequencies.
2. On the PNA menu, click **Sweep**, then **Sweep Type**. Select **Power Sweep**. Do NOT change the CW frequency on the Power Sweep dialog box. The mixer dialog box settings will not be automatically updated.

For more information, see [Conversion Compression](#).

## Input > LO Example

For the following single stage mixer:

- Output = 2 GHz
- LO = 3 GHz
- Diff (-) selected

Clicking **Calculate Input** could yield two Input frequencies:

Formula for **Diff**:

$$\text{Input} - \text{LO} = \text{Output}$$

Substitute our example values in the formula:

$$\text{Input} - 3\text{GHz} = 2 \text{ GHz}$$

Solving the formula can yield either:

$$\text{Input} = 5 \text{ GHz}$$

OR

$$\text{Input} = 1 \text{ GHz}$$

(Although  $1-3 = -2$  GHz, the analyzer displays the absolute value of the frequency.)

|                                    |                                                |                  |
|------------------------------------|------------------------------------------------|------------------|
| 5.000000000 GHz                    | 5.000000000 GHz                                | Calculate Output |
| 3.000000000 GHz                    | <input checked="" type="checkbox"/> Input > LO |                  |
| <input type="radio"/> +            | 8.000000000 GHz                                | Calculate Input  |
| <input checked="" type="radio"/> - | 2.000000000 GHz                                |                  |

**Check** - use the Input frequency (5 GHz) that is greater than LO (3 GHz)

|                                    |                                     |                  |
|------------------------------------|-------------------------------------|------------------|
| 1.000000000 GHz                    | 1.000000000 GHz                     | Calculate Output |
| 3.000000000 GHz                    | <input type="checkbox"/> Input > LO |                  |
| <input type="radio"/> +            | 4.000000000 GHz                     | Calculate Input  |
| <input checked="" type="radio"/> - | 2.000000000 GHz                     |                  |

**Clear** - use the Input frequency (1 GHz) that is less than LO (3 GHz)

## Configure Fixed Output Measurements

With PNA Revision 4.0, the Frequency Converter Application can make Fixed Output measurements. This requires that one or both LO (external sources) sweep in a synchronized manner with the Input.

Do the following to make a Fixed Output measurement with 1 LO:

1. Set Input to **Start/Stop**.
2. Set Input start and stop frequencies.
3. Set Output to **Fixed** - LO is automatically set to **Start/Stop**.
4. Set the Output frequency.
5. Click **Calculate LO** button
6. Click the LO **Not controlled** button to [Configure the External LO Source](#)


#### Notes:

- Although the PNA will allow you to leave LO as **Not Controlled**, this configuration will usually result in meaningless Fixed Output measurements.
- You can make Fixed Output Scalar and Vector measurements. However, only Scalar measurements can be calibrated.
- Because your Fixed Output measurement is controlling an external source, you may find that the measurement is very slow. Learn how to [speed up your Fixed Output measurement](#).

## Fractional Multiplier Examples

### Example 1

Use the LO fractional multiplier to replicate the action of the third-harmonic mixer so the PNA can accurately calculate the receiver frequency. The input and LO frequencies are known.

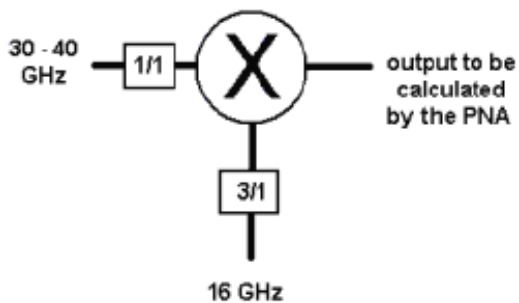

Enter these settings in the **Mixer Setup** dialog box:

- **Input Start Freq: 30 GHz**
- **Input Stop Freq: 40 GHz**
- **LO Fixed Freq: 16 GHz**
- Mixer-Product Selector: - (difference)
- LOs: 1
- LO fractional multiplier: 3/1
- INPUT fractional multiplier: 1/1




Click **Calculate Output**

Results:

- **Output Start Freq: 18 GHz**
- **Output Stop Freq: 8 GHz**

### Example 2

Use the fractional multipliers to tune the PNA receiver frequency to the second harmonic of the mixer's 14 GHz fundamental output. The input, LO, and output frequencies are known.

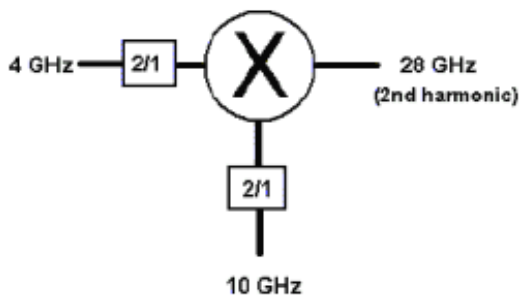

Enter these settings in the **Mixer Setup** dialog box:

- **Input Start Freq: 4 GHz**
- **Input Stop Freq: 4 GHz**
- **LO Fixed Freq: 10 GHz**
- Mixer-Product Selector: + (Sum) of the input and LO signals
- LOs: 1
- INPUT fractional multiplier = 2/1
- LO fractional multiplier = 2/1


Click **Calculate Output**

Results:

- **Output Start Freq: 28 GHz**
- **Output Stop Freq: 28 GHz**

### Example 3

Use the LO fractional multiplier to replicate the action of the divide-by-two mechanism inside the mixer package. Having done this, the PNA can accurately calculate the receiver frequency. The input and LO frequencies are known.

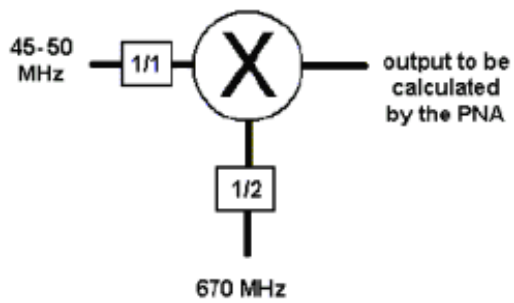

Enter these settings in the **Mixer Setup** dialog box:

- **Input Start Freq: 45 MHz**
- **Input Stop Freq: 50 MHz**
- **LO Fixed Freq: 670 MHz**
- Mixer-Product Selector: + (Sum) of the input and LO signals
- LOs: 1
- INPUT fractional multiplier = 1/1
- LO fractional multiplier = 1/2

Click **Calculate Output**

Results:

- **Output Start Freq: 380 MHz**
- **Output Stop Freq: 385 MHz**

## Configure an External LO Source

You can configure a LO source to be used when making either SCALAR or VECTOR Frequency Converter Application ([option 083](#)) measurements.


### How to Configure an External LO Source

1. [Create an FCA measurement](#)
2. Then either:

-  +
- or click **LO Control** in the [Configure Mixer](#) dialog box.

Learn more about using the [front panel interface](#)

**Note:** If an **External Source Not Found** error occurs, the Agilent I/O Library may no longer be running. To check, look in the Windows task bar of the PNA for the **IO** icon. If not present, restart the IO library. Click Start, Programs, Agilent I/O Libraries, IO Control.

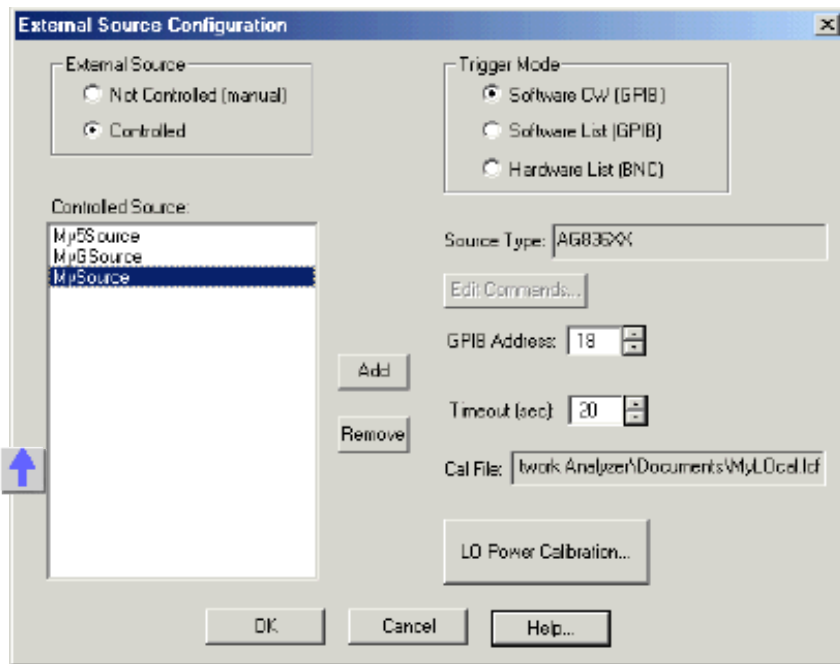

### External Source Configuration dialog box help

This dialog box is also used to configure external sources for Millimeter Wave Test Heads. [Learn more...](#)

There are currently no PNA programming commands to configure the external source.

Connect external sources to the PNA GPIB using either:

- The [Agilent 82357A USB/GPIB Interface](#) - **highly recommended** - allows for the use of a remote PC to control the PNA.
- The standard GPIB Interface - with the following limitations:

- The PNA cannot be controlled remotely as talker / listener over GPIB. First put the PNA in System Controller mode. [Learn how.](#)
- Available only on PNA releases 4.2 and later.

### External Source Configuration

**Not Controlled (manual)** The PNA does NOT control the external source. When this selection is made, all other settings in this dialog box do NOT apply.

**Controlled** The PNA controls the external sources using GPIB.

**Trigger Source** ONLY used when the external source is stepped (FCA Fixed output measurements).

---

**Note:** The PNA Trigger Source setting must NOT be set to EXTERNAL for any of the following selections.

---

See [SCPI](#) and [COM](#) examples of an SMC fixed output measurement.

**Software CW (GPIB)** Slowest method. The external source receives the CW frequency from the PNA over GPIB. This is the only selection available for generic (not listed), and Agilent 837X sources.

**Software List (GPIB)** The external source receives a list of CW frequencies from the PNA, then receives only trigger signals as required, over GPIB. Used ONLY for Agilent 836X sources.

**Hardware List (BNC)** Fastest method. The external source receives a list of CW frequencies from the PNA, then receives trigger signals as required from the PNA rear-panel BNC [Trigger](#) connectors.


---

**Note:** Hardware List is ALWAYS used for 2 External Sources driving [Millimeter Wave Heads](#).

---

The PNA will NOT respond to Manual Triggers in **Hardware List (BNC)** mode. The PNA trigger source must be set to INTERNAL. Then use the PNA [channel trigger settings](#) "Group" or "Single" to specify how the FCA measurement responds to internal triggers.

The sources must be connected in the following manner:

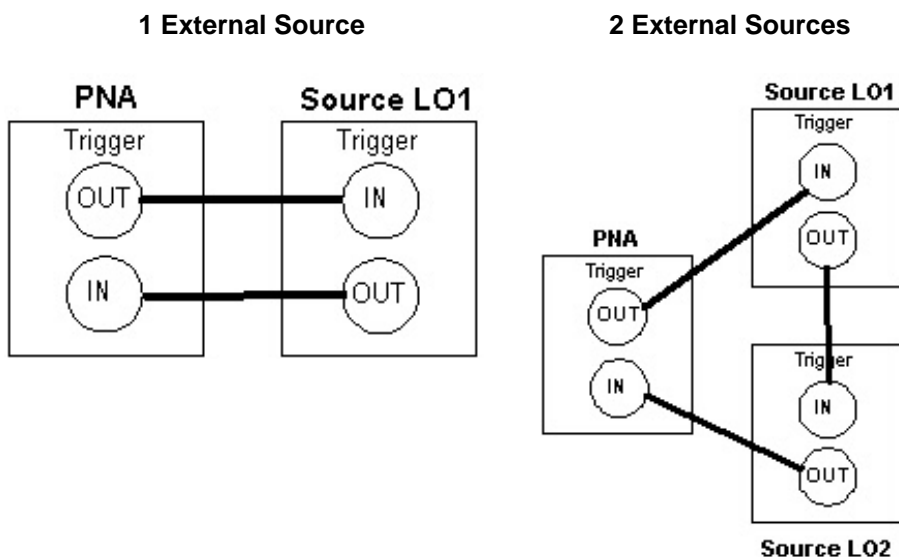


---

**Note:** The PNA checks communication with the sources the at the time of the first measurement sweep. If an error occurs, the PNA puts the channel in Hold trigger mode. You must fix the problem, then put the channel into either continuous or single sweep triggering to restart the measurement.

---

For more information, see:

- [Speeding Up Fixed Output SMC Measurements](#)

- PNA Trigger model

### Controlled Source

**Add** Displays the Add New Source dialog box.

**Remove** Removes an external source from your setup.

**Source Type** Shows the model number of the external source that is selected in the displayed list.

**Edit Commands** Only available with generic (non-Agilent) sources. Invokes the Edit Commands dialog box.


**GPIO Address** Sets the GPIO address of the selected external source.

**Timeout (sec)** Sets a time limit for the source to make contact with the PNA. If this time limit is exceeded, the PNA stops the measurement procedure and displays a diagnostic-type error message. If this occurs, check the connections of your PNA and source.

**Cal File:** Displays the calibration file that is in use with the selected external source. After configuring a source, a calibration must be performed to see the file. Enabling **Slope Offset** constitutes a calibration.

**LO Power Calibration** Displays the LO Power Calibration dialog box. A warning message appears stating that the changes you have made will be saved.

**Cancel** Closes the dialog box without saving changes (unless the **LO Power Calibration** button was pressed).

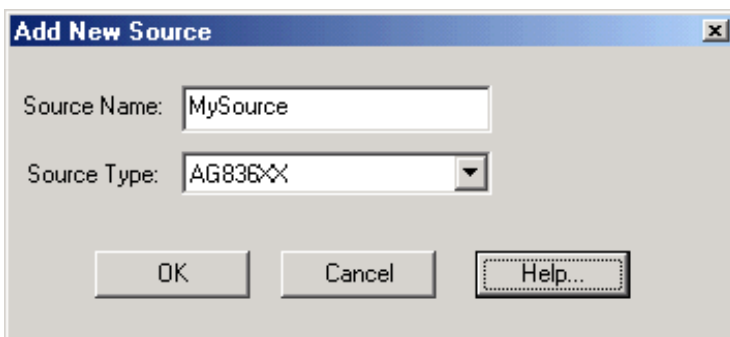


### Add New Source dialog box help

Allows you to add an external source. The new source appears in the list of sources displayed in the External Source Configuration dialog box.

**Source Name** Allows you to enter a name for your source.

**Source Type** Allows you to select a source type from the scrolling list.

To use an Generic external source (not listed) Select **AGGeneric**. This invokes the following **Generic Source Commands** dialog box.

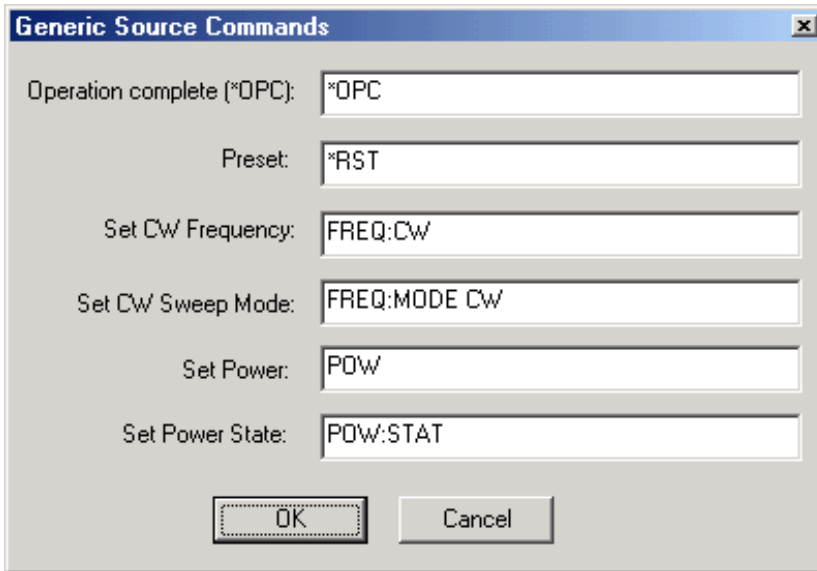

### Generic Source Commands dialog box help

Load the following SCPI commands that control the functions on your Generic (not listed) source.

**Operation Complete (\*OPC)** .


**Preset** Presets the source

**Set CW Frequency** Sets CW Frequency to value in Mixer Setup dialog

**Set CW Sweep Mode** Sets source sweep mode

**Set Power** Sets source power to value in Mixer Setup dialog

**Set Power State** Turns Power ON or OFF

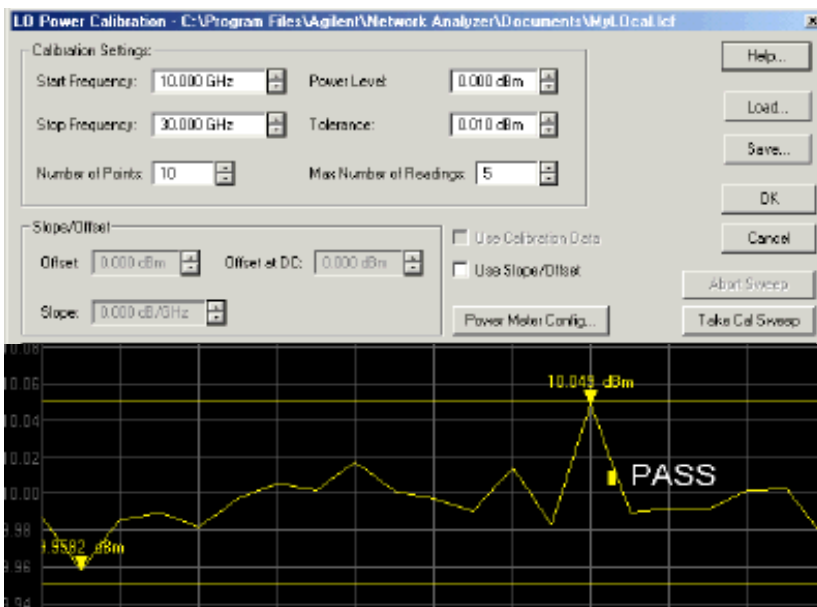

## LO Calibration dialog box help

Allows you to select, load, and save, calibration settings for your external source. Also, you can perform an LO calibration, set the slope/offset, and configure your power meter.

**Note:** The LO cal sweep, along with "tolerance" limit lines, is visible below the dialog box. Right click on the screen to access display settings.

### Calibration Settings

**Start Frequency** Sets the start frequency for the LO calibration.

**Stop Frequency** Sets the stop frequency for the LO calibration.

**Number of Points** Sets the number of data points that the power meter measures in the frequency range of the LO calibration.

**Power Level** Sets the power level for the LO calibration.

**Tolerance** Sets the maximum permissible deviation from the specified power level.

**Max Number of Readings** Sets the maximum number of iterative routines the PNA will perform to implement the power setting.

### Slope/Offset

**Offset** Sets the amount of offset power applied to each measurement point of the LO calibration frequency range. This power is offset from the power setting of the Slope feature.

**Offset at DC** Sets the amount of offset power applied at DC.

**Slope** Allows you to set the power slope (dB)/GHz. Compensates for cable and test fixture power loss by increasing the External LO output power over frequency.

**Use Calibration Data** Check to use the calibration data to correct your external source. The calibration data may come from a source calibration file (.lcf) that you have loaded, or from a new LO calibration.

**Use Slope/Offset** Check to apply the slope/offset settings to your external source. Using the slope/offset settings is a faster, but less thorough way to improve LO accuracy than performing an LO calibration. These settings can be used in addition to an LO calibration. For example, if you add an adapter in your LO path, you can use the slope/offset settings to compensate for the effects of the adapter rather than repeat the LO calibration.

**Power Meter Config** Displays the [Power Meter Settings dialog box](#).

**Abort Sweep** Immediately stops the calibration measurement.

**Take Cal Sweep** Starts the calibration measurement after a prompt to connect the power meter to the external source right at the DUT LO port.

**Load** Loads a source calibration file (.lcf) of your choice.

**Save** Saves your LO calibration data in a source calibration file (.lcf).


**Power Meter Settings** [See Source Power Calibration](#)

**Sensors** [See Source Power Calibration](#)

## External Leveling Circuitry that Uses a DC Preamplifier

**Note:** This circuitry will not work with E836x models; they do not have an External Leveling input on the rear panel.

The graphic below is a schematic diagram of **external leveling circuitry** (provided by the user) that uses a DC preamplifier. A preamplifier is recommended when the input power-level to the detector diode is less than -30 dBm.

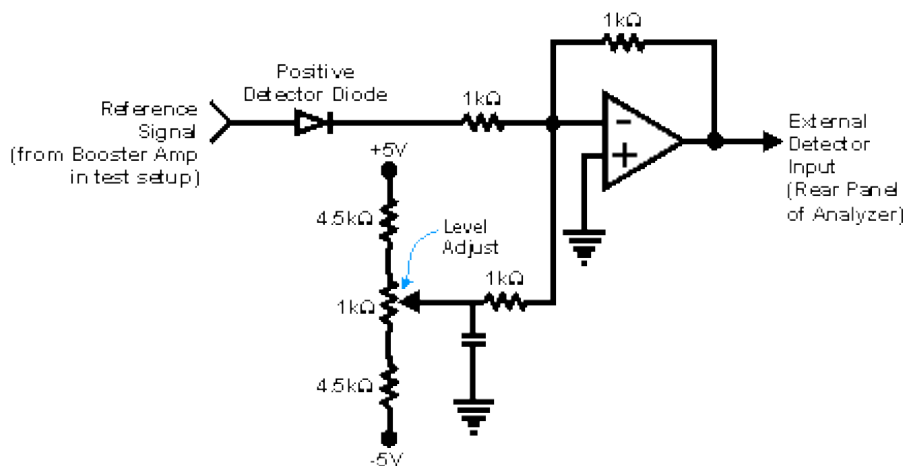

- The external leveling circuitry consists primarily of
  - A detector diode
  - An operational amplifier
- Changes in the power measured by the diode are detected by the operational amplifier circuit. This circuit regulates the voltage at the analyzer's External Detector Input, adjusting the analyzer's source power to achieve a flat response at the DUT on a real-time basis.
- For external leveling to work correctly, the voltage at the analyzer's External Detector Input must be between -0.002 mVDC and -6 VDC, depending on frequency and power level.
- Making too great a change in the reference-signal power can cause the external-leveling function to become ineffective due to the limited power-control range of the analyzer's source.



## High-Power Amplifier Measurements Using a PNA

---

High-power amplifiers have one or both of the following attributes:

- They require more input power than a standard analyzer can provide.
- They deliver more output power than a standard analyzer can measure.

**Click on a solution to learn to make measurements of high-power amplifiers:**

| Challenge                                                                      | Solution                                                                 |
|--------------------------------------------------------------------------------|--------------------------------------------------------------------------|
| Which test-set configuration does my PNA have?                                 | <a href="#">PNA test-set configurations</a>                              |
| DUT input-power is too low                                                     | <a href="#">Booster amplifiers in the test setup</a>                     |
| <b>E835xA, E880xA, and N338xA only:</b> Booster amplifier response is not flat | <a href="#">External leveling for booster amplifiers</a>                 |
| Phase-lock lost when using a booster amplifier                                 | <a href="#">Disable auto-frequency calibration</a>                       |
| Which measurement calibration do I use?                                        | <a href="#">Measurement calibration choices</a>                          |
| What calibration power levels do I use?                                        | <a href="#">Power-level recommendations for calibration</a>              |
| DUT output power is too high                                                   | <a href="#">Components that reduce DUT output power</a>                  |
| Will my calibration standards withstand high power?                            | <a href="#">Calibration standards that withstand high power</a>          |
| Thermal variations occur in my test setup                                      | <a href="#">Thermal requirements for DUTs and loads</a>                  |
| DUT has an Automatic Gain Control (AGC) loop                                   | <a href="#">Stimulus-sweep recommendation for a DUT with an AGC loop</a> |
| What procedure do I use to measure high-power amplifiers?                      | <a href="#">Procedure for Measuring High-Power Amplifiers</a>            |

**Note:** Many of the external components shown in the test set-up configurations of this tutorial are available from Agilent Technologies. For example, Agilent sells couplers, power splitters, and attenuators. Go to <http://www.agilent.com/find/accessories> and use the search function to locate information on components you may want to purchase. You can also get [Agilent technical support](#) by telephone or fax.

### PNA Test-Set Configurations

**[Here's how to identify your PNA.](#)**

Configuration graphics of PNA test sets:

| <b>PNA without Configurable Test Set</b> | <b>PNA with <u>Configurable Test Set</u></b> |
|------------------------------------------|----------------------------------------------|
| <u>E835xA</u>                            | <u>E835xA, Option 015</u>                    |
| <u>E880xA</u>                            | <u>E880xA, Option 014</u>                    |
| <u>N338xA</u>                            | <u>N338xA, Option 014</u>                    |
| <u>E836xA/B</u>                          | <u>E836xA/B, Option 014</u>                  |
| <u>N5230A</u>                            | <u>N5230A, Option 225, or 425, or 525</u>    |
| N5230 Opt 240                            | N5230 Opt 245                                |
|                                          | <u>N5250A</u>                                |

### **Booster Amplifiers in the Test Setup**

If your DUT requires more input power to be tested accurately than the analyzer can provide, you need to provide a booster amplifier in your test setup. (See your analyzer's power range in the [Technical Specifications](#).) However, using a booster amp may limit the types of testing and calibration you can perform. Also, your booster amplifier may not provide a consistent power level to your DUT over the frequency range of interest. If your booster amplifier requires you to provide a leveling loop, see [External Leveling for Booster Amplifiers](#), available only on models **E835xA, E880xA, and N338xA**.

Configuration graphics for using booster amp circuitry:

| <b>Configuration</b>                             | <b>PNA without Configurable Test Set<sup>1</sup></b>                                                                                    | <b>PNA with <u>Configurable Test Set</u></b>                                                                                                                                                                                        |
|--------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>One Booster Amp</b>                           | <u>E835xA</u> <sup>2</sup><br><u>E880xA</u> <sup>2</sup><br><u>N338xA</u> <sup>2</sup><br><u>E836xA/B</u> <sup>2</sup><br><u>N5230A</u> | <u>E835xA, Option 015</u> <sup>3</sup><br><u>E880xA, Option 014</u> <sup>3</sup><br><u>N338xA, Option 014</u> <sup>3</sup><br><u>E836xA/B, Option 014</u> <sup>3</sup><br><u>N5230, Option 225, or 425, or 525</u><br><u>N5250A</u> |
| <b>One Booster Amp &amp; One Reverse Coupler</b> | <u>E835xA</u> <sup>3</sup>                                                                                                              |                                                                                                                                                                                                                                     |
| <b>Two Booster Amps</b>                          | <u>E835xA</u> <sup>4</sup>                                                                                                              | <u>E835xA, Option 015</u><br><u>E880xA, Option 014</u><br><u>N338xA, Option 014</u> <sup>5</sup><br><u>E836xA/B, Option 014</u><br><u>N5230A, Option 225, or 425, or 525</u><br><u>N5250A</u>                                       |

1 You can choose from other booster amplifier configurations by purchasing the Configurable Test Set upgrade. For E835xA analyzers, order Option 015. For all other analyzers, order Option 014. **See PNA Options**.

**Limitations** (footnotes 2 - 5):

2 • Allows only a Thru Response Cal for boosted forward transmission ( $S_{21}$ ) measurements.

- Allows only a 1-Port Reflection Cal or Open/Short Response Cal for non-boosted reverse reflection ( $S_{22}$ ) measurements.

- Reverse *boosted-power* measurements are not possible unless the booster amplifier is relocated.

- Reflection measurements on Port 1 or reverse transmission measurements are not possible. The signal is blocked by the booster amplifier.

3 Reverse *boosted-power* measurements are not possible unless the booster amplifier is relocated.

4 None.

5 **N338xA Option 014 only:** Reverse boosted-power measurements are not possible from Port 3. This is because Port 3 does not have Source Out and Coupler Thru channels.

## Disable Automatic Frequency Calibration when using Booster Amps.

When using a booster amplifier, or whenever removing a front-panel jumper cable to provide a signal to the internal reference receiver, you may see a phase-lock lost indication. This can occur if you use a narrow-band filter or coupler in your test setup.

If phase-lock lost indication occurs, the PNA will automatically re-calibrate the tuning curve of the internal source. To prevent the PNA from re-calibrating itself, disable the Automatic Frequency Calibration while the PNA is still phase locking correctly.

To do this, Click **System**, then point to **Configure**, then click **SICL/GPIB**. At the prompt, type **DIAG:AUTOCAL OFF**.

The PNA may still lose phase-lock outside of the pass band of your coupler or filter, but the PNA will not try to re-calibrate itself.

---

**Note:** For best performance, the reference receiver power must be 22dB (+/-5dB) below the power at the test port.

---

## External Leveling for Booster Amplifiers

---

Note: External leveling is not possible with the E8361A, E8362A/B, E8363A/B, E8364A/B, N5230, N5250.

---

If the boosted response of your DUT is not as flat as you expect, it may be attributed to the output of your external booster amp. If the output has ripple across the frequency band of interest, your DUT will amplify that ripple. You can add your own external leveling circuitry to compensate for poor flatness of an external booster amplifier in your test setup.

### How do I Determine If I Need to Use External Leveling with my Booster Amplifier?


Use your analyzer to measure the peak-to-peak ripple of your booster amplifier. If the level of peak-to-peak ripple is unacceptable for the measurement accuracy you require, use external leveling.

---

**Note:** Be sure to calibrate before measuring the peak-to-peak ripple of your booster amplifier. Calibration will prevent noise (if present) from varying the look of your measurement during each sweep of the analyzer.

---

As shown in the following graphic, a booster-amplifier without external leveling may have ripple that causes DUT response ripple.

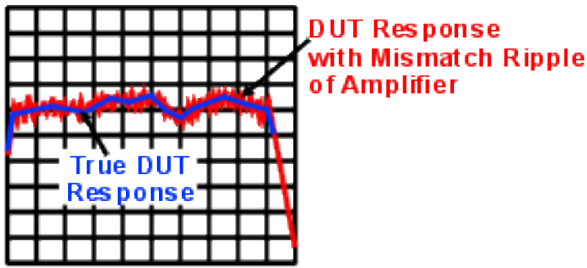

Some causes of booster-amplifier ripple:

- Low quality booster amplifier (poor match or flatness)
- Noisy power-supply voltage for booster amplifier
- Saturated booster amplifier

### What Configurations Do I Use For External Leveling?

Note: External leveling is not possible with the E8361A, E8362A/B, E8363A/B, E8364A/B.

Configuration graphics for using external leveling circuitry:

| External Leveling Configuration                 | Standard Analyzers                              | Option 014 and 015 Analyzers                                                        |
|-------------------------------------------------|-------------------------------------------------|-------------------------------------------------------------------------------------|
| One Booster Amplifier                           | <u>E835xA</u><br><u>E880xA</u><br><u>N338xA</u> | <u>E835xA, Option 015</u><br><u>E880xA, Option 014</u><br><u>N338xA, Option 014</u> |
| One Booster Amplifier and a Reverse Coupler     | <u>E835xA</u>                                   |                                                                                     |
| Two Booster Amplifiers and Two Reverse Couplers | <u>E835xA</u>                                   |                                                                                     |
| Two Booster Amplifiers                          |                                                 | <u>E835xA, Option 015</u><br><u>E880xA, Option 014</u><br><u>N338xA, Option 014</u> |

### Power Levels for External Leveling

The analyzer's test port power should be maintained between **+10 dBm and -15 dBm** for proper phase lock and ALC (automatic level control) operation. If no external DC preamplifier is used at the DC output of the detector diode, the power applied to the input of the detector diode should be maintained between **+10 dBm and -20 dBm**. This power range is necessary to achieve an adequate DC output from the detector diode for proper ALC operation. A negative-output detector diode should be used, such as an Agilent 3330C (you can find information about this detector diode at <http://www.agilent.com/find/accessories>.) The DC output of the detector is connected directly (using a coaxial cable) to the analyzer's rear panel "Ext Detector Input."

### More information about the external leveling circuitry:

- The detector diode's output voltage, applied to the analyzer's External Detector Input, adjusts the source power to achieve a flat response at the DUT on a real-time basis.
- For external leveling to work correctly, the voltage at the analyzer's External Detector Input must be between -0.002 mVDC and -6 VDC, depending on frequency and power level.

- Making too great a change in the reference-signal power can cause the external leveling function to become ineffective due to the limited power-control range of the analyzer's source.

View [external leveling circuitry that uses a DC preamplifier](#) (recommended when the input power-level to the detector diode is less than -20 dBm).

---

**Note:** When performing a [calibration](#), keep the source-leveling process active, just as it will be during the measurement.

---

### Which Analyzer Menu Choices Do I Select for External Leveling?

---

Note: External leveling is not possible with the E8361A, E8362A/B, E8363A/B, E8364A/B.

---

#### E835xA:

1. Select the **Sweep** menu.
2. Select **Sweep Setup**. Select the **External ALC** checkbox.
3. Select the **Channel** menu.
4. Select **Power**. In the **Attenuator Control** section of the dialog box, clear the **Auto** checkbox.

#### E880xA and N338xA only:

1. Select the **Sweep** menu.
2. Select **Sweep Setup**. Select the **External ALC** checkbox.

Find more information about using external leveling at <http://www.tm.agilent.com>. Click "Library" and use the search function to search for "ALC."

### Measurement Calibration Choices

---

**Note:** Calibration should be performed with all hardware in place. For example, include any booster amplifiers, cables, attenuators, or couplers that will be used when measuring the DUT. For more calibration information, refer to [Measurement Calibration Choices](#).

---

**CAUTION:** When using an open or a short during calibration, be sure that the incident power level is low enough so that the reflected signal doesn't exceed the maximum input to the analyzer's receivers.

---

Calibration choices are determined by the measurement configuration you use.

The following are configuration graphics and calibration choices for high-power measurements:

| Measurement Direction                                 | PNA without Configurable Test Set                                                   | PNA with Configurable Test Set                                                                                                                                    | Calibration Choices                                                                              |
|-------------------------------------------------------|-------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------|
| <b>Forward</b>                                        | <u>E835xA</u>                                                                       | <u>E835xA, Opt 015</u><br><u>E880xA, Opt 014</u><br><u>N338xA, Opt 014</u><br><u>E836xA/B, Opt 014</u><br><u>N5230A, Opt 225, or 425, or 525</u><br><u>N5250A</u> | 2-Port Calibration <sup>1</sup><br>1-Port Calibration <sup>2</sup>                               |
| <b>Forward (single-port cal only)</b>                 | <u>E835xA</u><br><u>E880xA</u><br><u>N338xA</u><br><u>E836xA/B</u><br><u>N5230A</u> |                                                                                                                                                                   | Thru Response <sup>3</sup><br>1-Port Reflection <sup>4</sup><br>Open/Short Response <sup>4</sup> |
| <b>Forward and reverse</b>                            | <u>E835xA</u>                                                                       | <u>E835xA, Opt 015</u><br><u>E880xA, Opt 014</u><br><u>N338xA, Opt 014</u><br><u>E836xA/B, Opt 014</u><br><u>N5230A, Opt 225, or 425, or 525</u><br><u>N5250A</u> | 2-Port Calibration <sup>5</sup><br>1-Port Calibration <sup>6</sup>                               |
| <b>Forward and reverse (non-boosted measurements)</b> | <u>E835xA</u><br><u>E880xA</u><br><u>N338xA</u><br><u>E836xA/B</u><br><u>N5230A</u> |                                                                                                                                                                   | 2-Port Calibration <sup>7</sup><br>1-Port Calibration <sup>8</sup>                               |

1 (TRL or SOLT) For forward high-power transmission and reflection measurements. Also for reverse non-boosted transmission and reflection measurements.

2 (Thru Response, 1-Port Reflection, or Open/Short Response) For forward high-power transmission or reflection measurements. Or, for reverse non-boosted transmission or reflection measurements.

3 For forward high-power transmission measurements.

4 For reverse non-boosted reflection measurements.

5 (TRL or SOLT) For forward and reverse high-power transmission and reflection measurements.

6 (Thru Response, 1-Port Reflection, or Open/Short Response) For forward or reverse high-power transmission or reflection measurements.

7 (TRL or SOLT) For forward and reverse non-boosted transmission and reflection measurements.

8 (Thru Response, 1-Port Reflection, or Open/Short Response) For forward or reverse non-boosted transmission or reflection measurements.

## Power Level Recommendations for Calibration

For greatest measurement accuracy, calibrate at the highest possible power below the onset of receiver compression. This power level depends on the frequency of the response being measured. (See your analyzer's [Technical Specifications](#) for the maximum input power to a receiver.)

**Analyzers with front-panel jumpers only:** Receiver power levels can be measured with a power meter where your external circuitry connects to:


- Rcvr A In channel or (for E835xA) A In channel
- Rcvr A In channel or (for E835xA) B In channel

During calibration (when the DUT is removed) adjust the power to get a power level at the receivers that safely minimizes receiver compression. During measurements (when the DUT is installed) adjust the power to maintain the safe power level at the receivers.

## Components that Reduce DUT Output Power

Maximum input power at the analyzer's receivers must not be exceeded. (See your analyzer's [Technical Specifications](#) for the maximum input power to a receiver.) If your DUT has a high output-power level, it must be reduced to a level that can be safely handled by the analyzer's receivers. As shown in the following graphic, when testing a CDMA base-station amplifier, some or all of the following components are configured to reduce amplifier output power:

- An external high-power **coupler** can be installed at the output of the amplifier. A special **load** that can dissipate high power is used to terminate the through-arm of the coupler.
- An external high-power **attenuator** can be attached to the analyzer's input port.

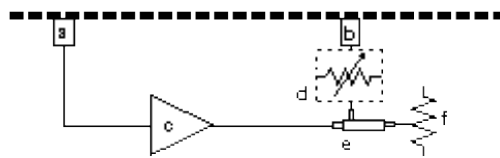

| Item | Description                                                                                                                                                                                                                                                   | Item | Description                            |
|------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------|----------------------------------------|
| a    | PORT 1                                                                                                                                                                                                                                                        | e    | Directional coupler, customer supplied |
| b    | PORT 2                                                                                                                                                                                                                                                        | f    | Load, customer supplied                |
| c    | CDMA base station amplifier, customer supplied                                                                                                                                                                                                                |      |                                        |
| d    | Variable attenuator (optional), customer supplied. (If your E835x PNA is equipped with Option 015, or any other PNA is equipped with Option 016, it has <u>receiver attenuation</u> and does not require external attenuation. See <u>Analyzer Options</u> .) |      |                                        |

**To protect your analyzer's receiver from too much input power**, follow these steps to determine values of an external attenuator (or an internal receiver attenuator, if equipped with Option 015 or 016) or coupler and load (or both).

1. Determine the maximum power out of the amplifier [Ex: 40 dBm].
2. Subtract 15 dB (the coupling-factor value of the directional coupler inside the analyzer) [Ex: 40 dBm - 15dBm = 25 dBm].
3. Subtract the power level required at the receiver [Ex: 25 dBm - (-10 dBm)].
4. The result is the appropriate value of the external attenuator (or an internal receiver attenuator, if equipped with Option 015 or 016) or coupler and load or both [Ex: 35 dB].

---

**Note:** Refer to the specifications for the coupler, load, and attenuator to ensure they have adequate power-handling capability.

---

Find more information about testing CDMA amplifiers at <http://www.tm.agilent.com>. Click "Library" and use the search function to search for CDMA amplifiers.

## Calibration Standards that Withstand High Power

- The line, open, short, and thru standards are not a problem with high-power levels since they do not dissipate any energy.
- The load dissipates energy. To prevent causing damage to the load, read its specifications to verify it can handle the power level.

---

**CAUTION:** When using an open or a short during calibration, be sure that the incident power level is low enough so that the reflected signal does not exceed the maximum input to the analyzer's receiver. See your analyzer's Technical Specifications for the damage level of a receiver.

---

If you are using an Electronic Calibration (ECal) Module, refer to its specifications for maximum input power.

## Thermal Requirements for DUTs and Loads

Thermal conditions during the high-power measurement should also be considered for accurate measurements. For example:



- The high-power DUT may respond very differently at various temperatures. The tests should be done when the amplifier is at the desired temperature.
- The load should be allowed to temperature-stabilize if its impedance characteristics change significantly versus temperature.

### Stimulus-Sweep Recommendation for a DUT with an AGC Loop

It is recommended that you set the analyzer to sweep across only one frequency band if you are testing an amplifier with an AGC loop. This will require a separate measurement across each of the required frequency bands, but it will ensure the safety of your amplifier.

Turning off the amplifier's source power is a problem for amplifiers (DUTs) containing an AGC (Automatic-Gain Control) loop. The problem occurs when the analyzer's source power sweeps through its band-crossings. The analyzer keeps power constant while sweeping or retracing if only **one** frequency band is used. If switching frequency bands, the analyzer blanks, or turns off, the source power as it sweeps or retraces.

When the analyzer's source power is blanked, the AGC loop of the amplifier tries to compensate by increasing its gain to keep the output power level constant. When blanking stops and the sweep begins again, the analyzer restores its signal, and suddenly there is power again at the input of the amplifier, which has ramped-up its gain. If the AGC loop cannot respond quickly enough, the momentary high output power can damage or destroy the amplifier under test and the analyzer's receiver.

View your analyzer's [frequency band crossings](#).

### Procedure for Measuring High-Power Amplifiers

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).


---

1. Select the correct analyzer configuration for your DUT and your measurement requirements. Do not connect the DUT yet.
2. Preset the analyzer.
3. If necessary, adjust the analyzer's source power:
  - Set the analyzer's source power to be in the linear region of the amplifier's output response (typically 10 dB below the 1 dB compression point).
  - Select an external attenuator (if needed) so the amplifier's output power will be sufficiently attenuated to avoid causing receiver compression or damage to the analyzer.
4. Select the desired measurement.
5. Connect the DUT.
6. Select the settings for the DUT.
7. Remove the DUT and perform a measurement [calibration](#). Be sure to include any booster amplifiers, cables, attenuators, or couplers that will be used when measuring the DUT.
8. Save the instrument state to memory.
9. Reconnect the [DUT](#).
10. Scale the displayed measurement for optimum viewing and use markers to read-out measurement results.

11. Print the data or save it to a disk.


## Diagram: (E835x) Basic Configuration

Explore the graphic with your mouse.

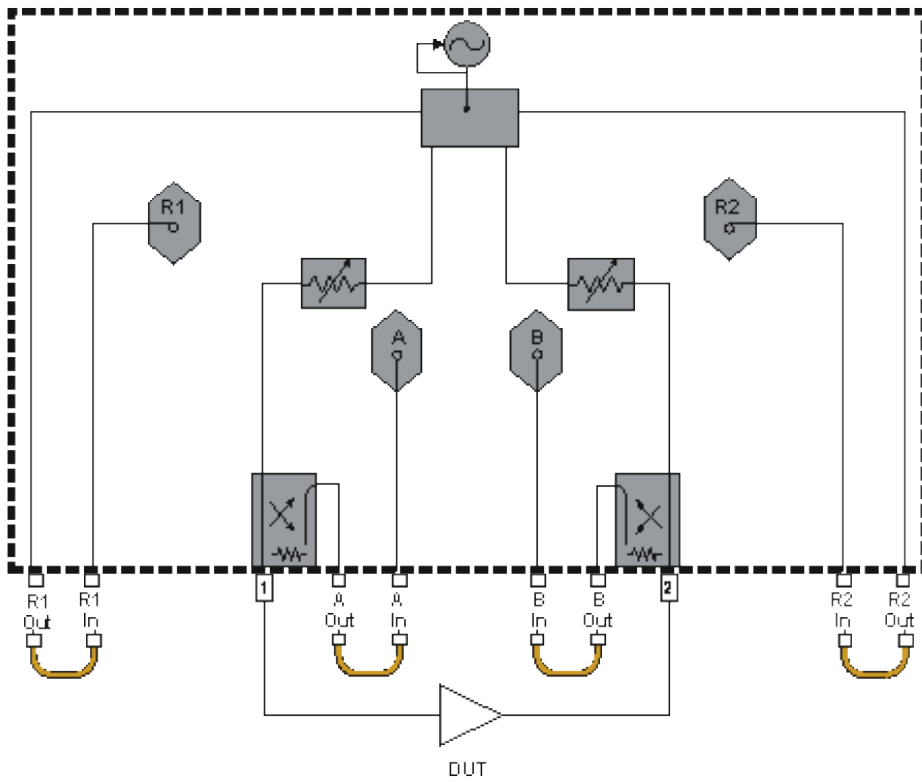


# Diagram: (E835x) Configuration for High-Power Measurements in the Forward Direction (Single-Port Cal Only)

Explore the graphic with your mouse.

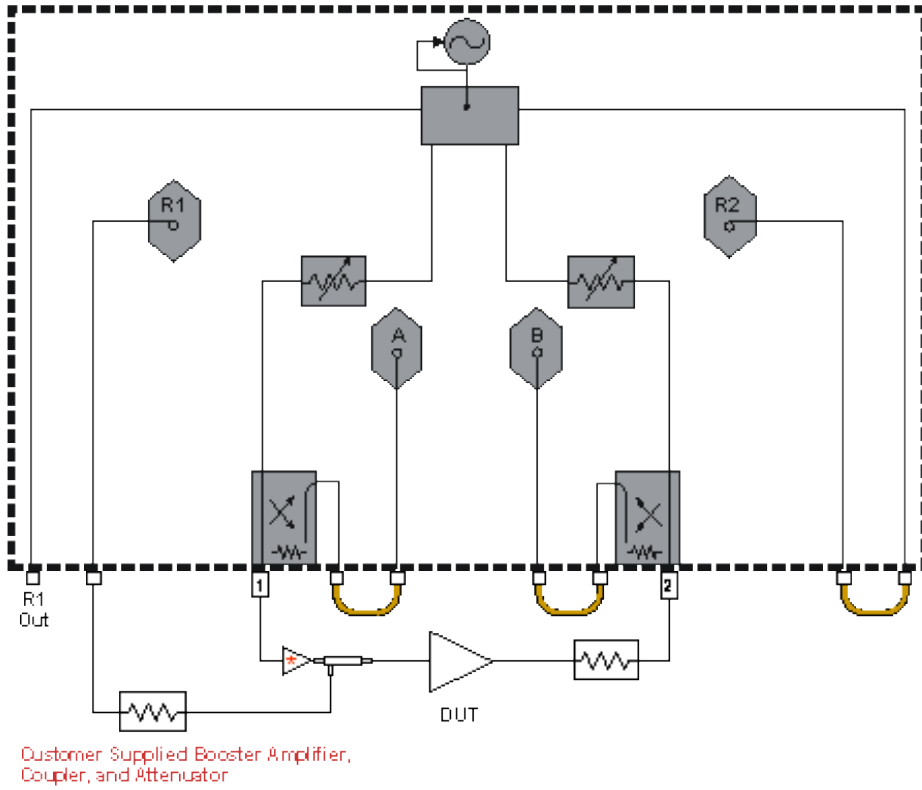


# Diagram: (E835x) Configuration for High-Power Measurements in the Forward Direction (2-Port Cal)

Explore the graphic with your mouse.

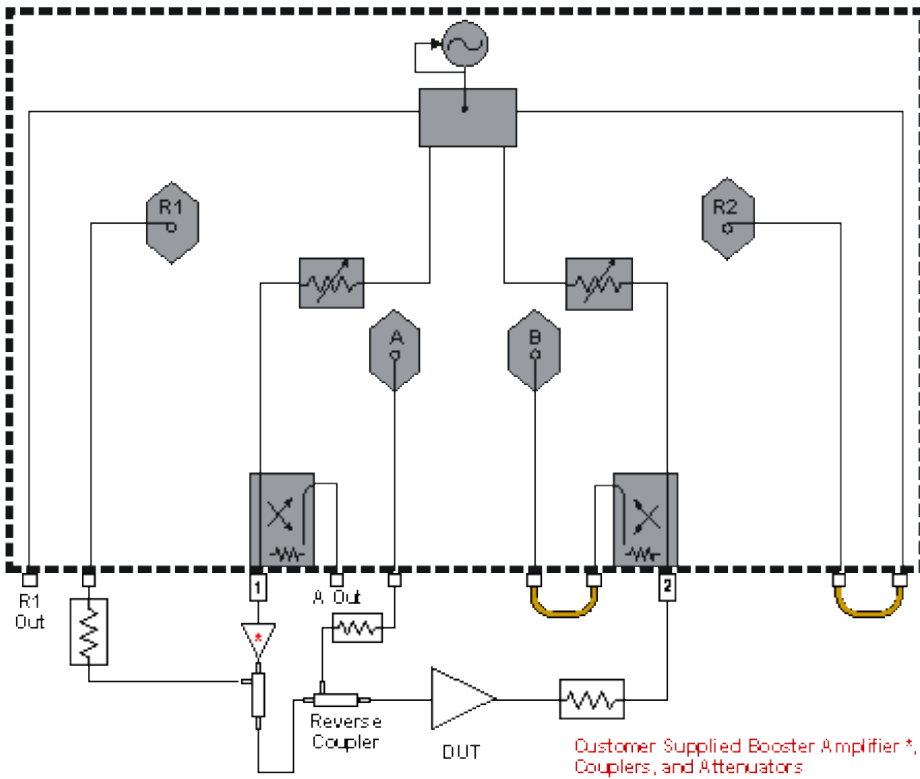

# Diagram: (E835x) Configuration for Non-Boosted High-Power Measurements in both Forward & Reverse Directions


Explore the graphic with your mouse.

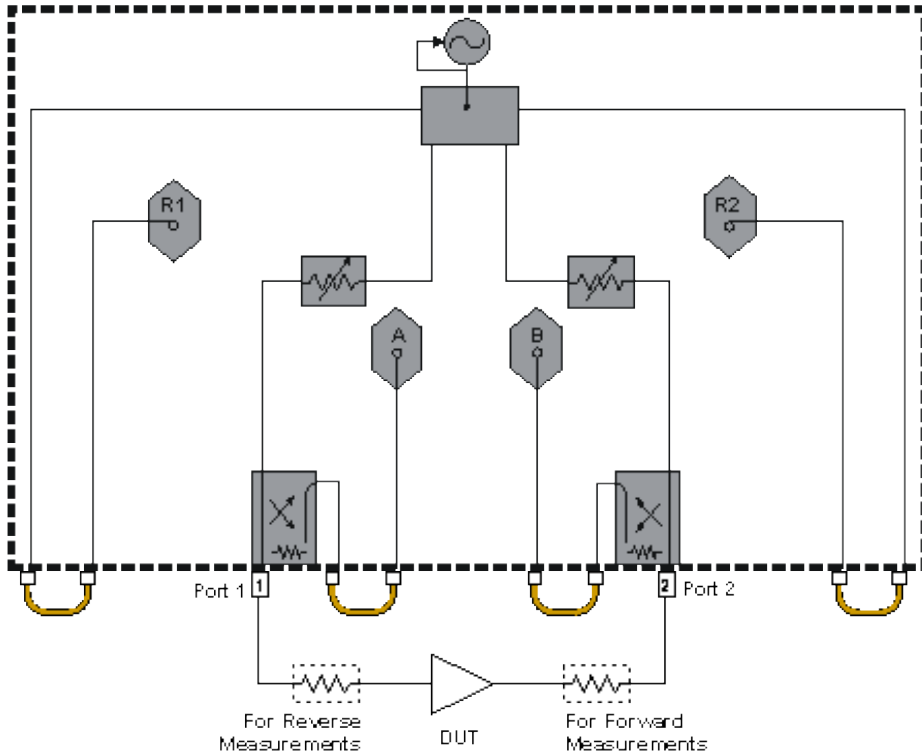

Customer Supplied Attenuator - Location dependent on direction of measurement

# Diagram: (E835x) Configuration for High-Power Measurements in both the Forward & Reverse Directions (2-Port Cal)


Explore the graphic with your mouse.

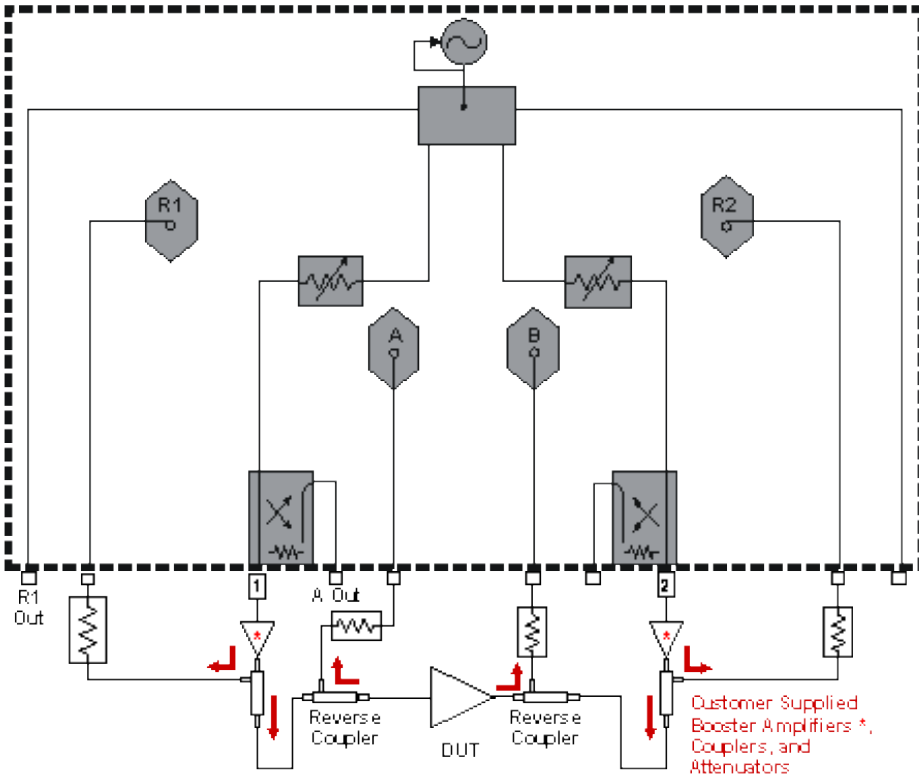

## Diagram: (E835x) Configuration using One Booster Amplifier

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, a forward coupler, and an attenuator.

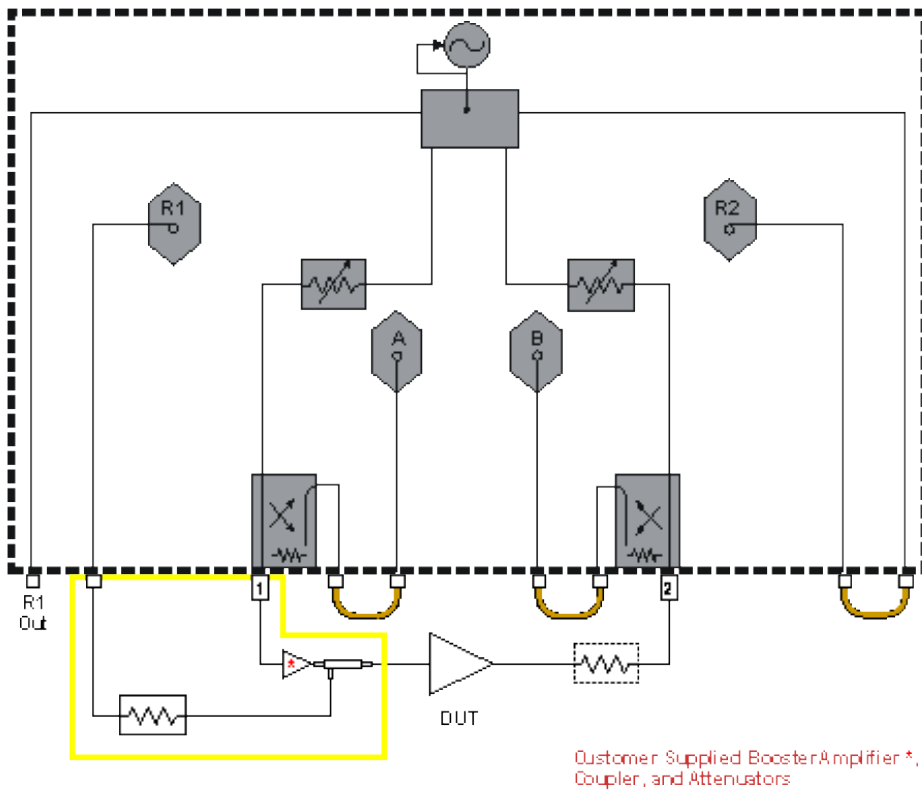








## Diagram: (E835x) External Leveling using One Booster Amplifier

Explore the graphic with your mouse.


**Note:** the circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, forward coupler, power splitter, two attenuators, and a negative detector diode.

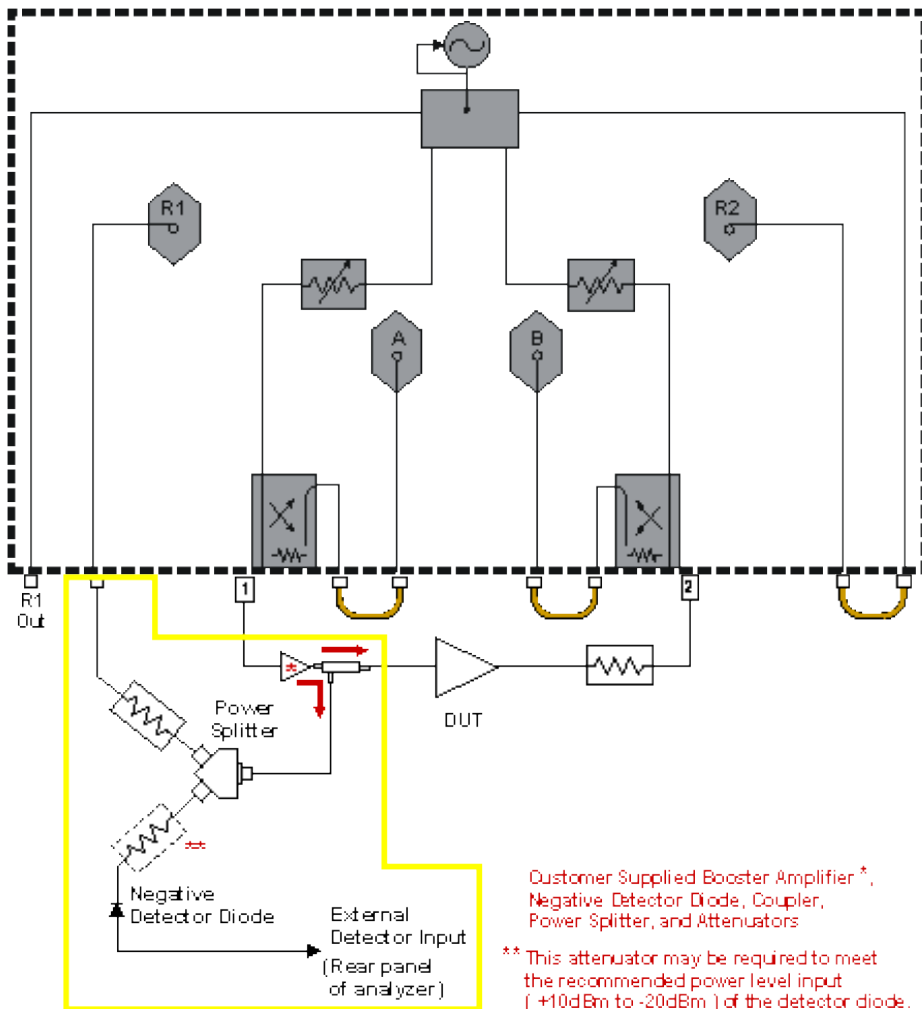

## Diagram: (E835x) External Leveling using One Booster Amplifier and a Reverse Coupler

Explore the graphic with your mouse.


**Note:** the circuitry inside the yellow lines contains the following components supplied by you - a booster amp, forward coupler, reverse coupler (allows S11 measurements), power splitter, three attenuators, and a negative detector diode.

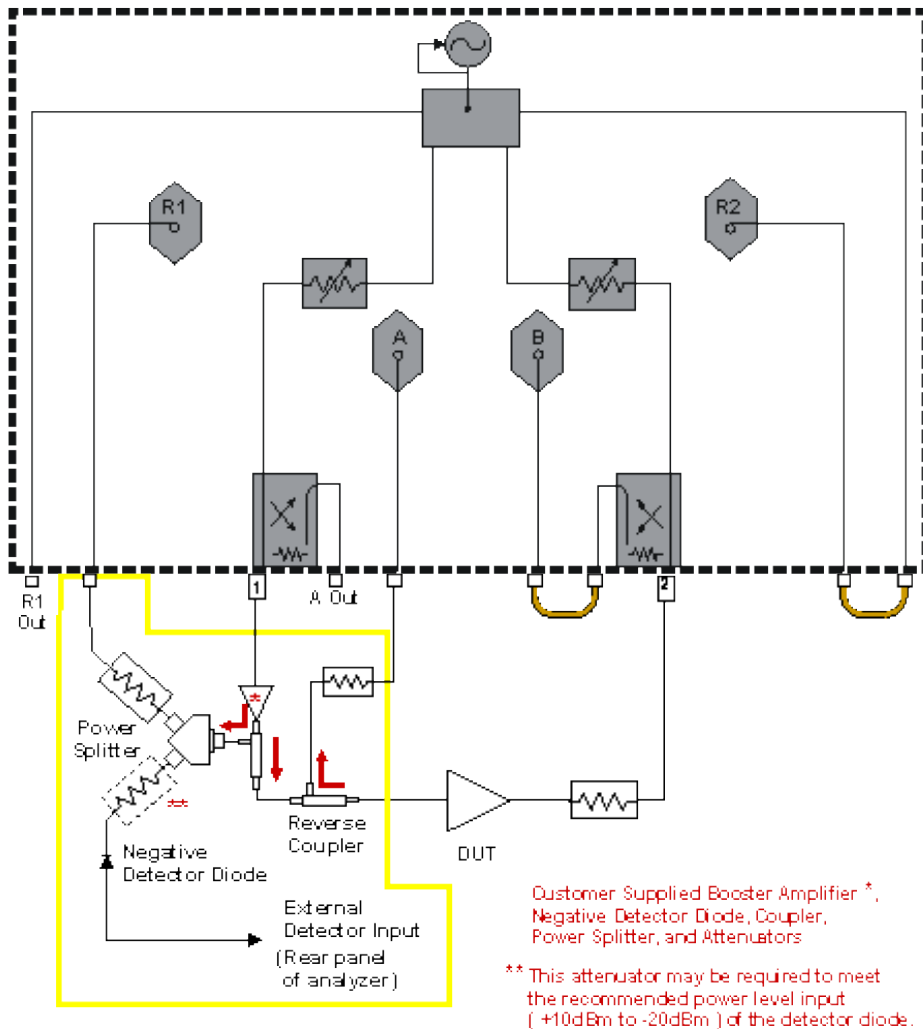


## Diagram: (E835x) External Leveling using Two Booster Amplifiers and Two Reverse Couplers

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains the following components supplied by you - 2 booster amps, 2 forward couplers, 2 reverse couplers (allow S11 and S22 measurements), 2 power splitters, 6 attenuators, and a negative detector diode.

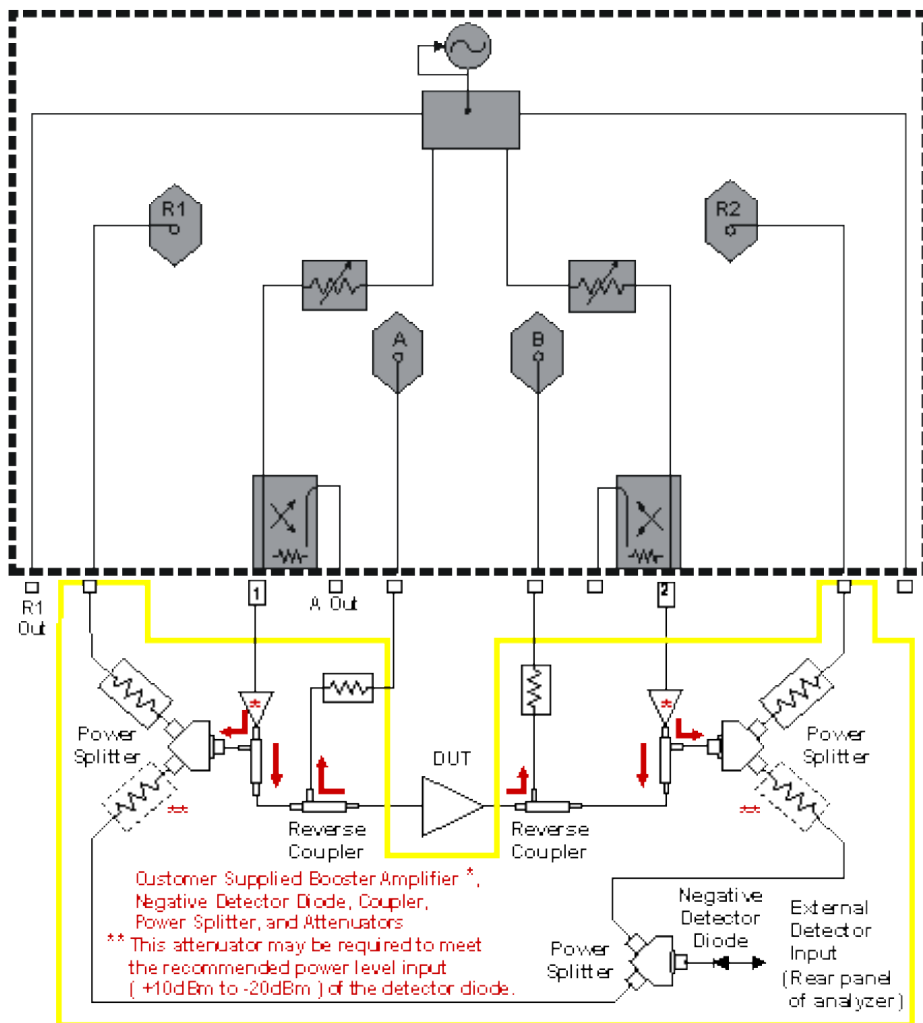


## Diagram: (E835x) Measuring Calibration Power Levels

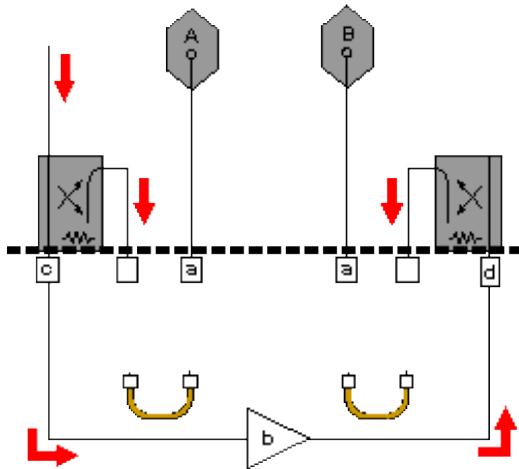

| Item | Description                                                                  |
|------|------------------------------------------------------------------------------|
| a    | Measure the receiver input power where your external circuitry connects here |
| b    | DUT, customer supplied                                                       |
| c    | PORT 1                                                                       |
| d    | PORT 2                                                                       |


## Diagram: (E835x, Option 015) Basic Configuration

Explore the graphic with your mouse.

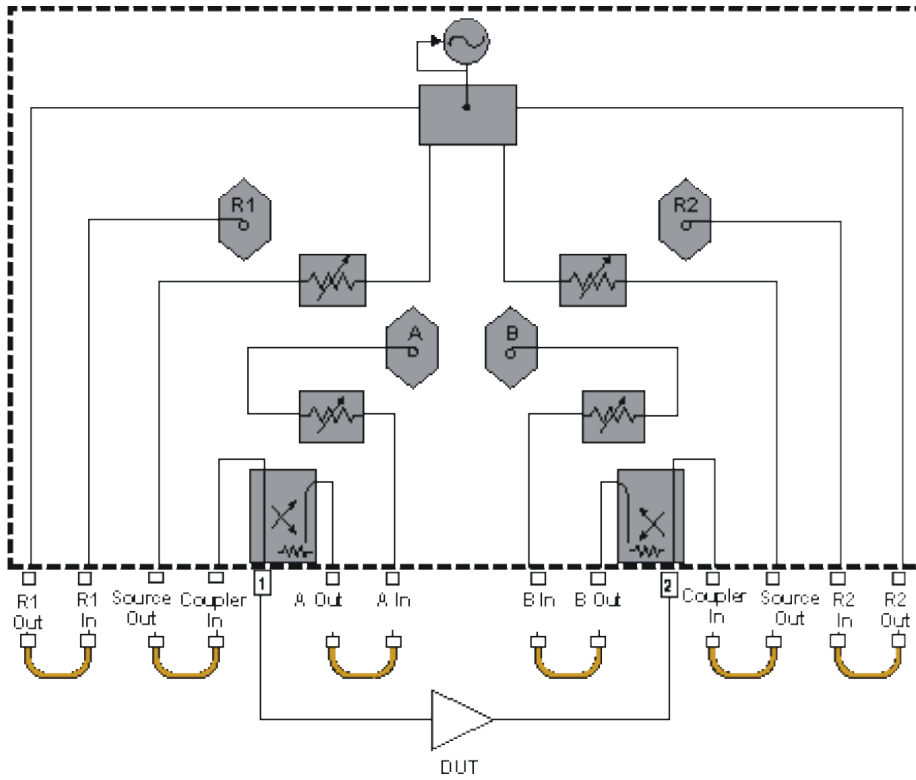

# Diagram: (E835xA, Option 015) Configuration for High-Power Measurements in the Forward Direction


Explore the graphic with your mouse.

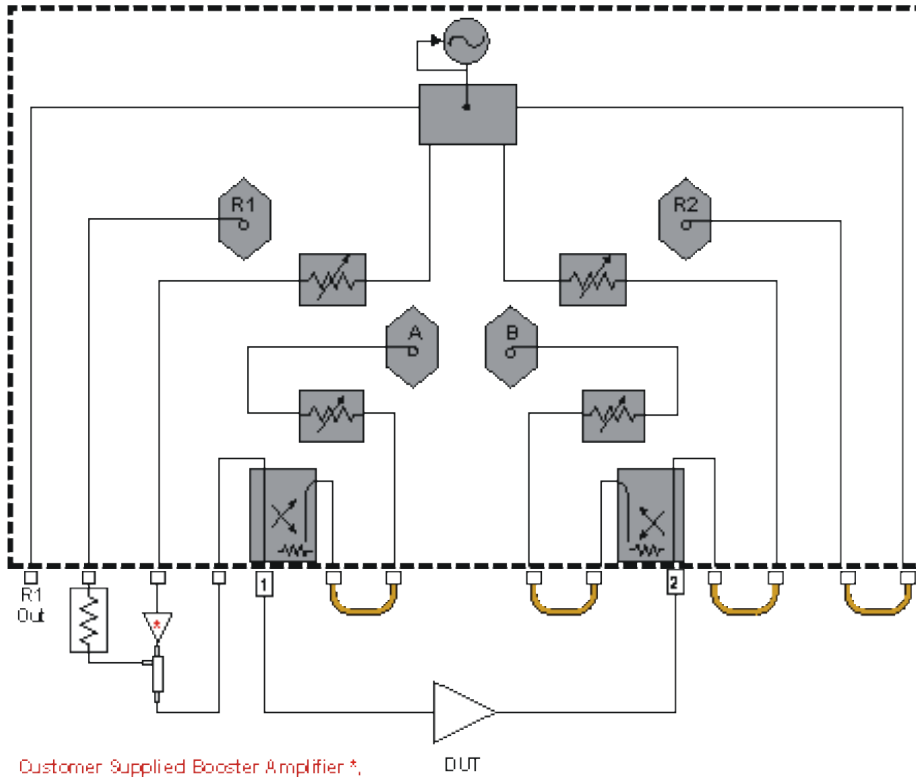




# Diagram: (E835xA, Option 015) Configuration (with an Isolator) for High-Power Measurements in the Forward Direction

Explore the graphic with your mouse.

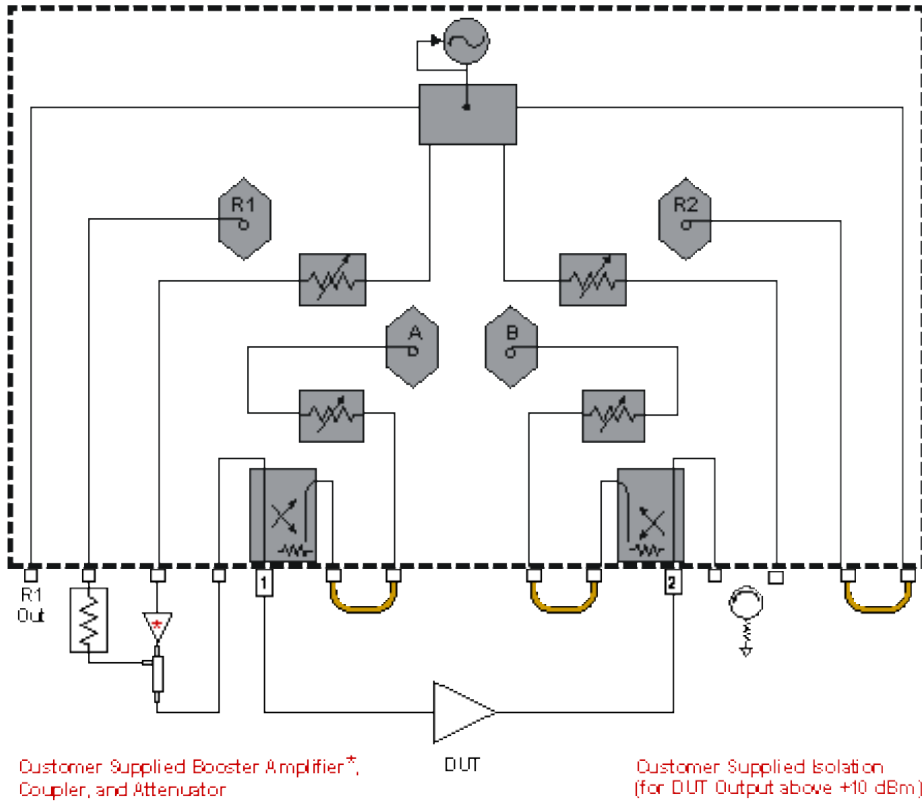

# Diagram: (E835xA, Option 015) Configuration for High-Power Measurements in both Forward & Reverse Directions


Explore the graphic with your mouse.

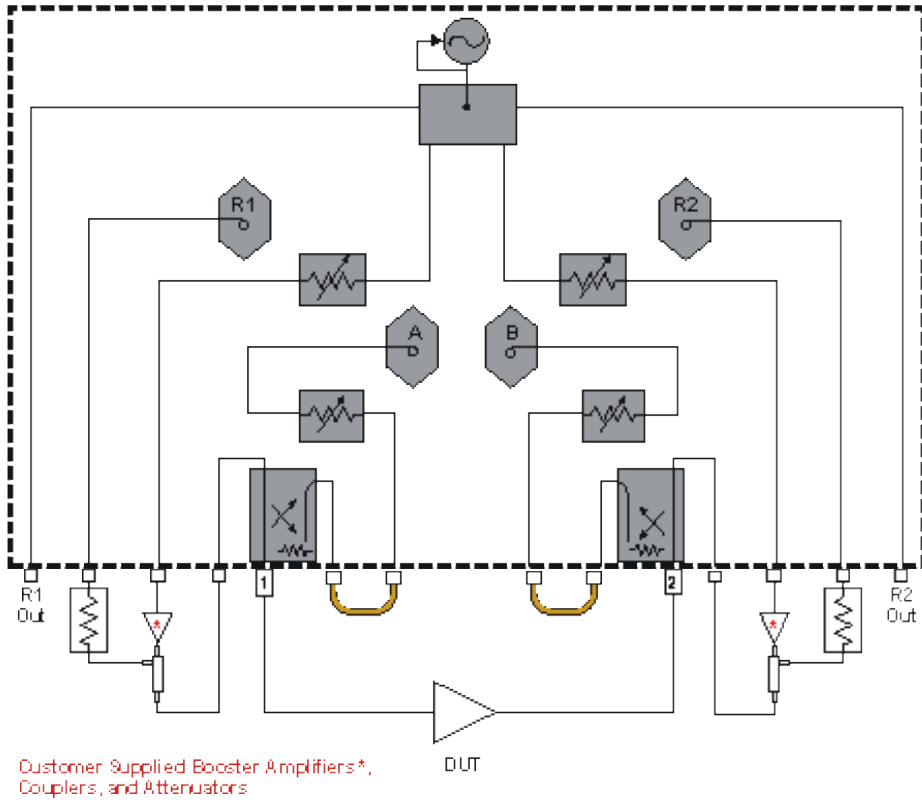

## Diagram: (E835x, Option 015) Configuration using One Booster Amplifier

Explore the graphic with your mouse.


**Note:** the circuitry inside the yellow lines contains the following components supplied by you: a booster amplifier, a forward coupler, and an attenuator.

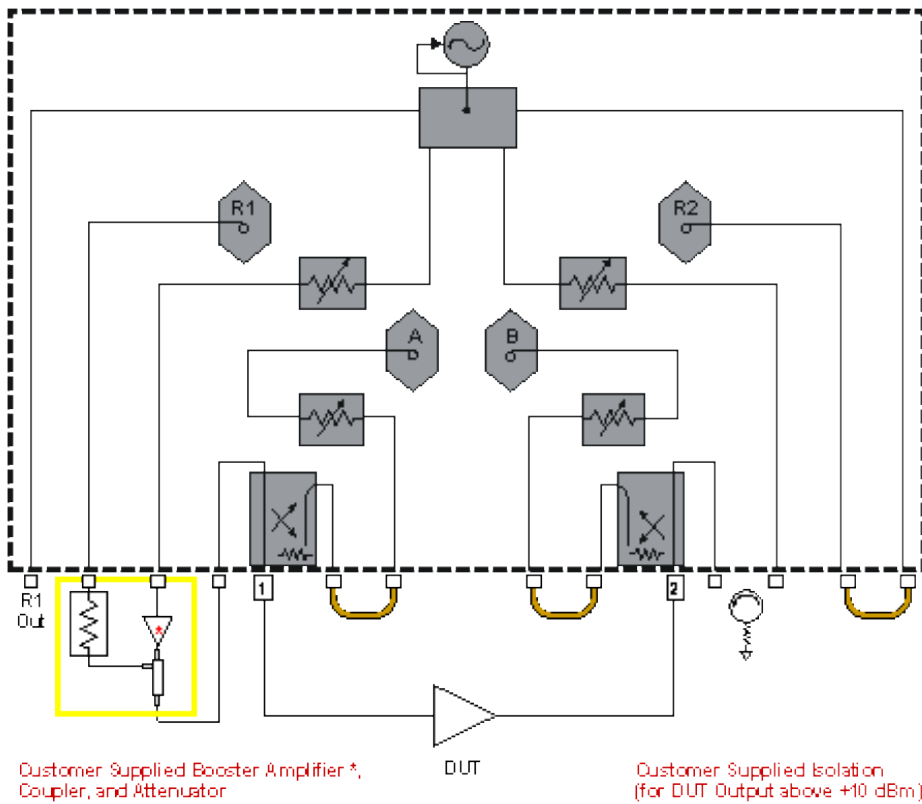

## Diagram: (E835xA, Option 015) Configuration Using Two Booster Amplifiers

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains the following components supplied by you: two booster amps, two forward couplers, and two attenuators.

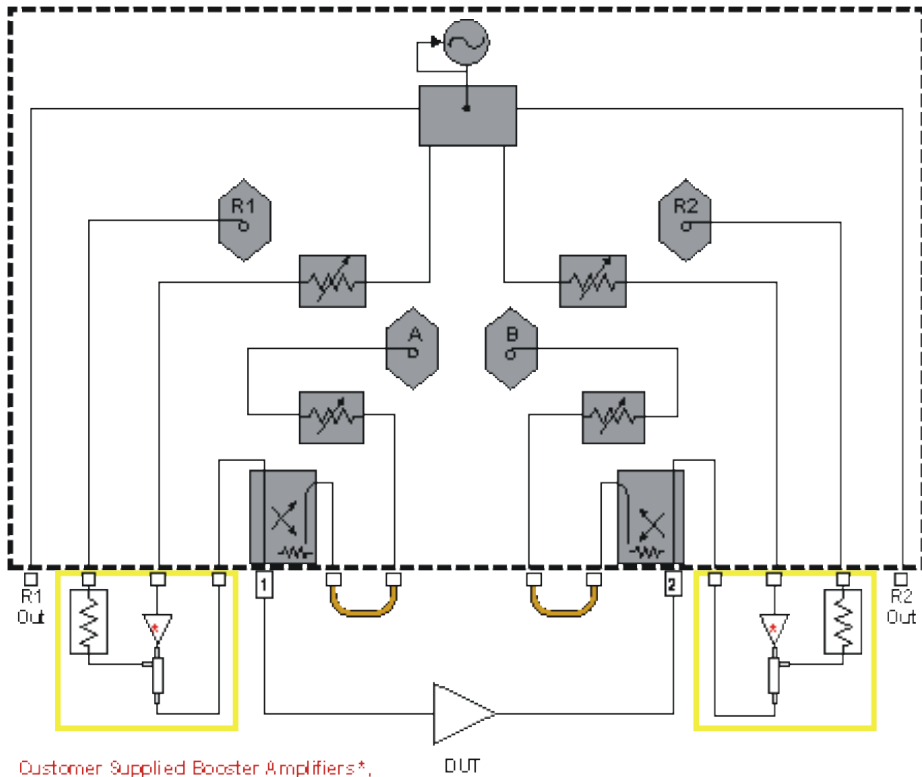


Customer Supplied Booster Amplifiers\*,  
Couplers, and Attenuators

## Diagram: (E835x, Option 015) External Leveling using One Booster Amplifier

Explore the graphic with your mouse.


**Note:** the circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, a forward coupler, power splitter, attenuators, and a negative detector diode.

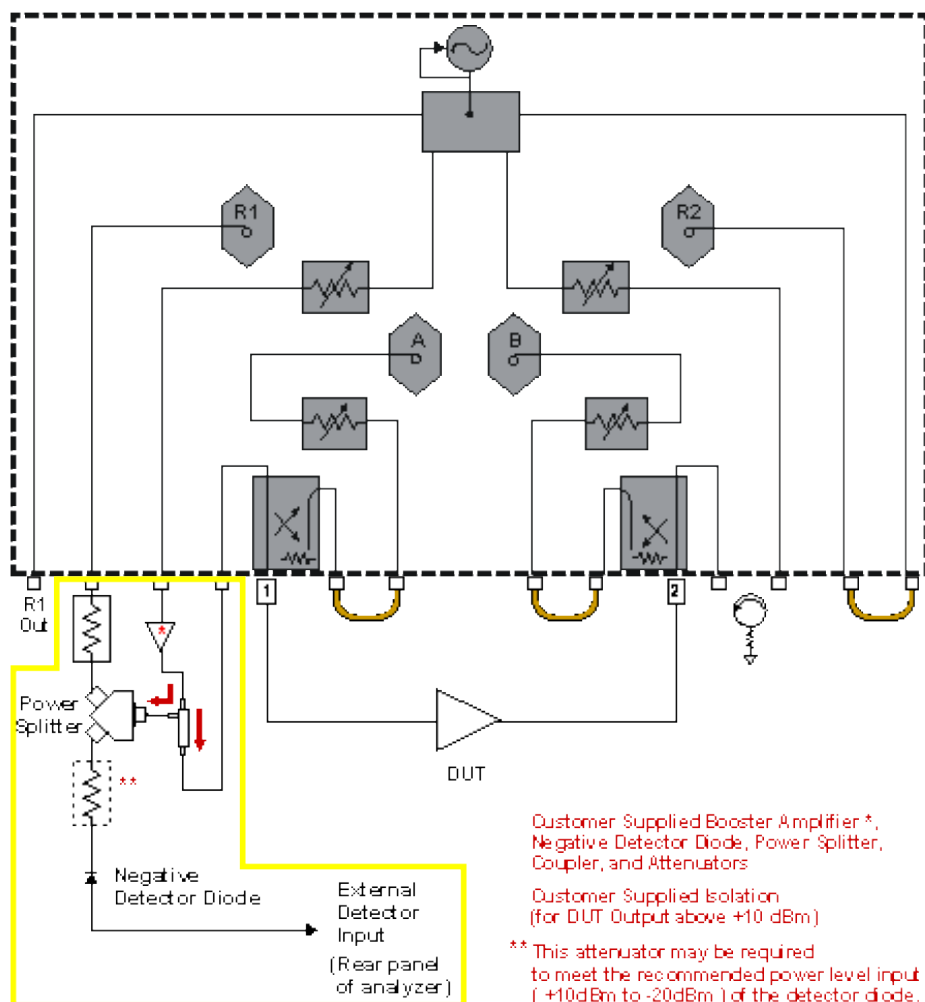

## Diagram: (E835xA, Option 015) External Leveling using Two Booster Amplifiers

Explore the graphic with your mouse.


**Note:** the circuitry inside the yellow lines contains the following components supplied by you: two booster amps, two forward couplers, attenuators, three power splitters, and a negative detector diode.

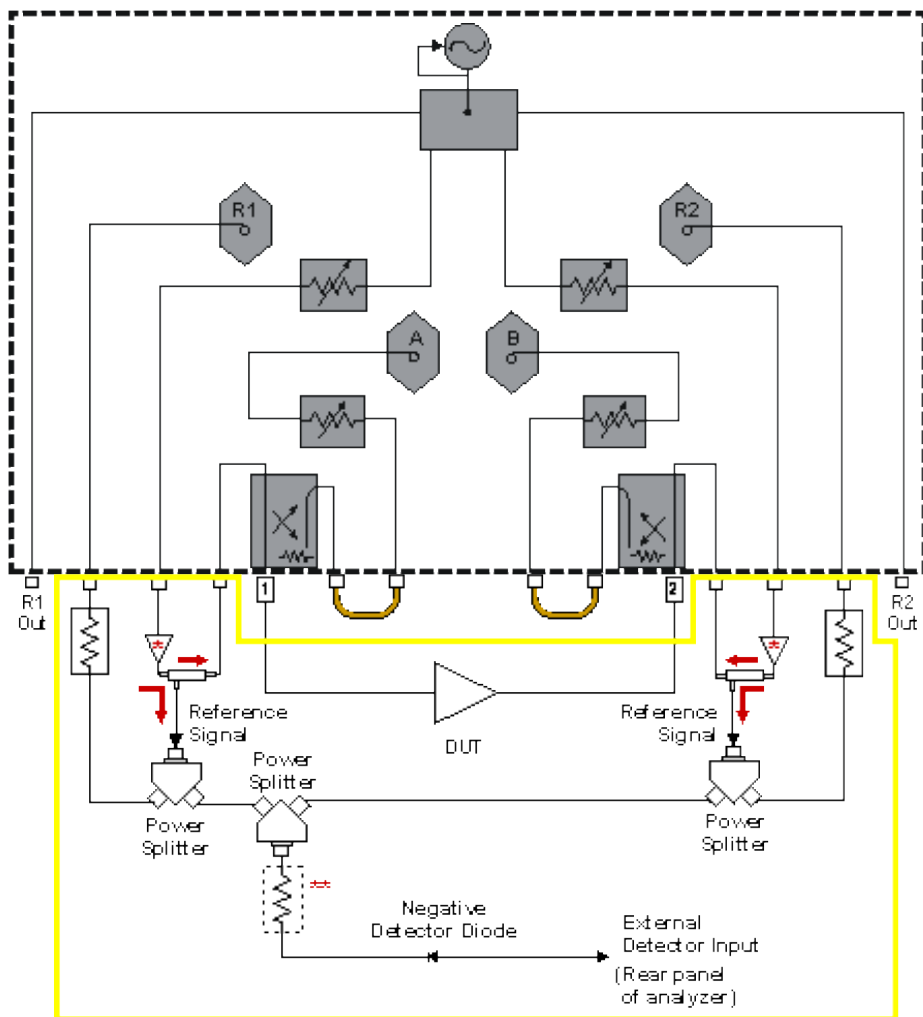

Customer Supplied Booster Amplifiers\*, Negative Detector Diode, Couplers, Power Splitters and Attenuators

\*\* This attenuator may be required to meet the recommended power level input (+10dBm to -20dBm) of the detector diode.


# Diagram: (E835xA, Option 015) Measuring Calibration Power Levels

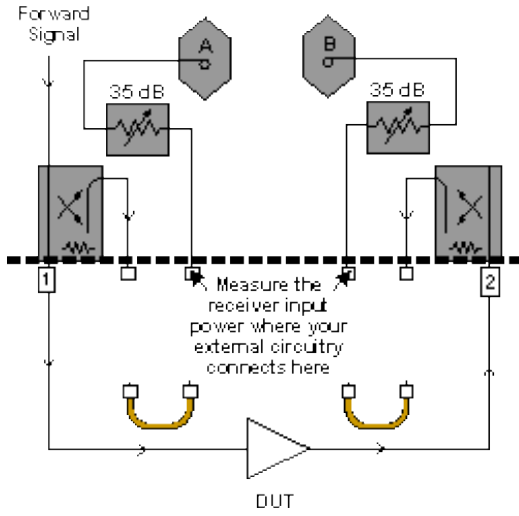

## Diagram: Basic Configuration

- E8361A, E8362A/B, E8363A/B, E8364A/B
- N5230A

Explore the graphic with your mouse.

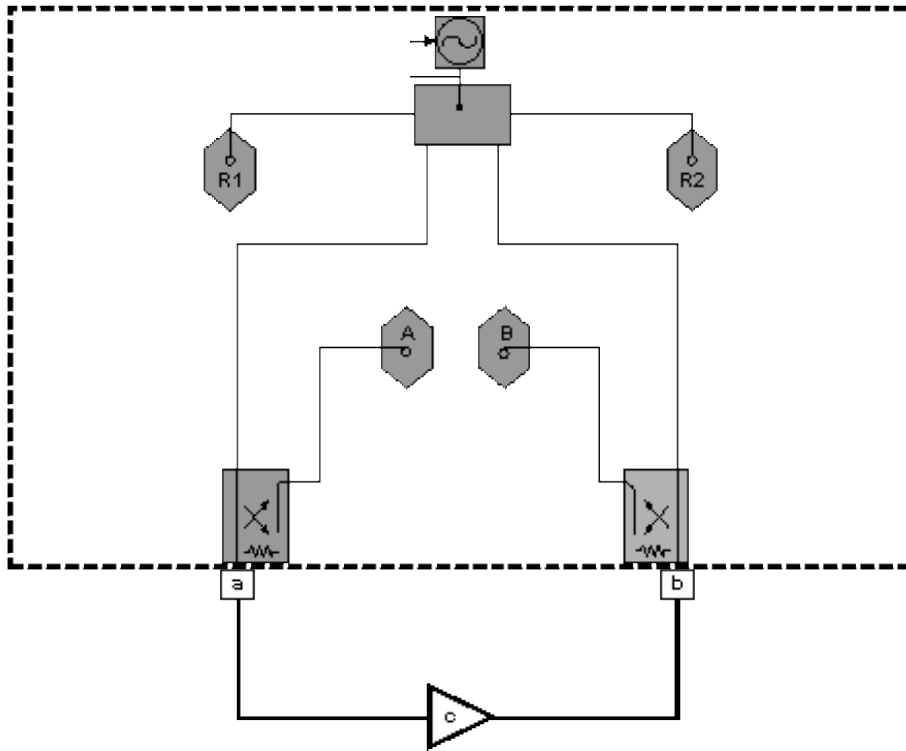


| Item | Description                  |
|------|------------------------------|
| a    | PORT 1                       |
| b    | PORT 2                       |
| c    | DUT,<br>customer<br>supplied |



## Diagram: Configuration for High-Power Measurements in the Forward Direction (Single-Port Cal Only)

- E8361A, E8362A/B, E8363A/B, E8364A/B
- N5230A

Explore the graphic with your mouse.

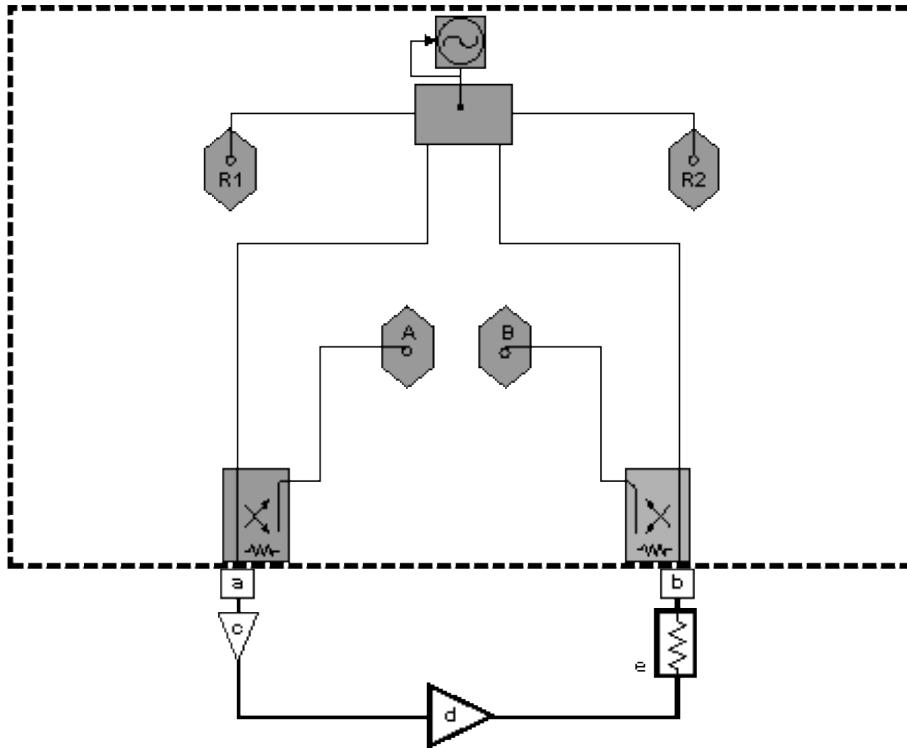


| Item | Description                          | Item | Description                                              |
|------|--------------------------------------|------|----------------------------------------------------------|
| a    | PORT 1                               | e    | Attenuator (for forward measurements), customer supplied |
| b    | PORT 2                               |      |                                                          |
| c    | Booster amplifier, customer supplied |      |                                                          |
| d    | DUT, customer supplied               |      |                                                          |

## Diagram: Configuration for Non-Boosted High-Power Measurements in both Forward and Reverse Directions

- E8361A, E8362A/B, E8363A/B, E8364A/B
- N5230A

Explore the graphic with your mouse.

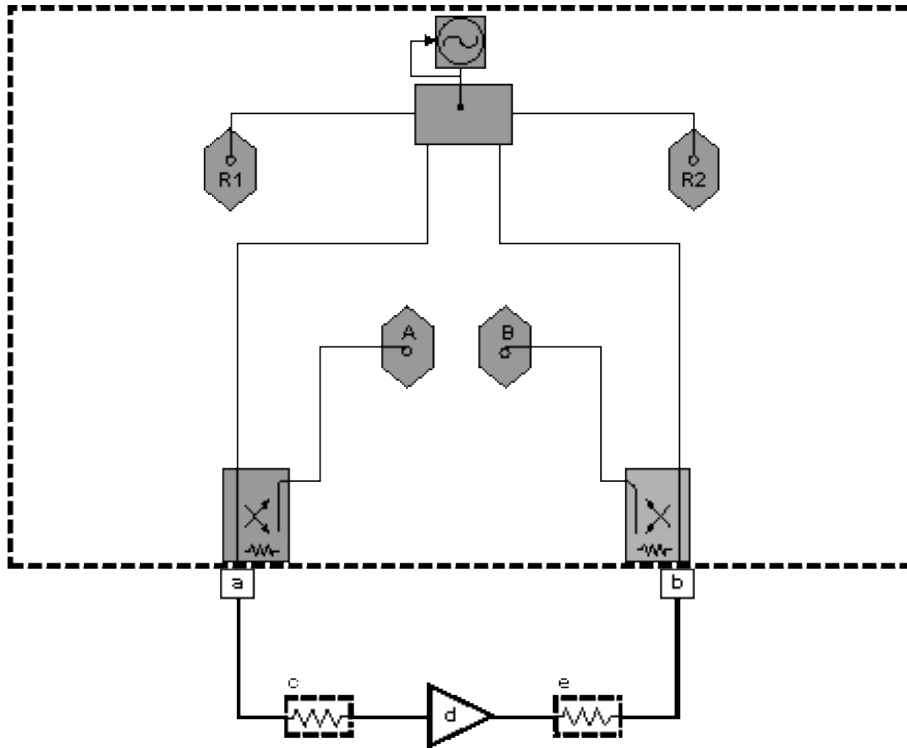


| Item | Description                                              | Item | Description                                              |
|------|----------------------------------------------------------|------|----------------------------------------------------------|
| a    | PORT 1                                                   | e    | Attenuator (for forward measurements), customer supplied |
| b    | PORT 2                                                   |      |                                                          |
| c    | Attenuator (for reverse measurements), customer supplied |      |                                                          |
| d    | DUT, customer supplied                                   |      |                                                          |

## Diagram: Configuration using a Booster Amp

- E8361A, E8362A/B, E8363A/B, E8364A/B, N5230A
- N5230A

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains a booster amplifier supplied by you.

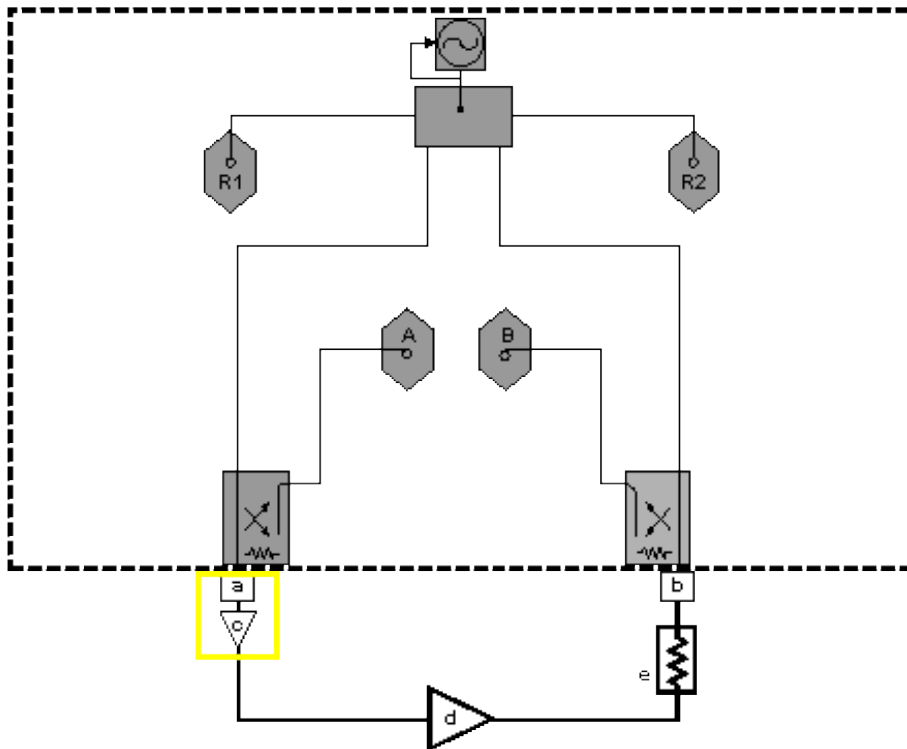


| Item | Description                          | Item | Description                                              |
|------|--------------------------------------|------|----------------------------------------------------------|
| a    | PORT 1                               | e    | Attenuator (for forward measurements), customer supplied |
| b    | PORT 2                               |      |                                                          |
| c    | Booster amplifier, customer supplied |      |                                                          |
| d    | DUT, customer supplied               |      |                                                          |

## Diagram: Basic Configuration

- E8361A, E8362A/B, E8363A/B, E8364A/B, Option 014
- N5230A Option 225, or 425, or 525
- N5250A


Explore the graphic with your mouse.

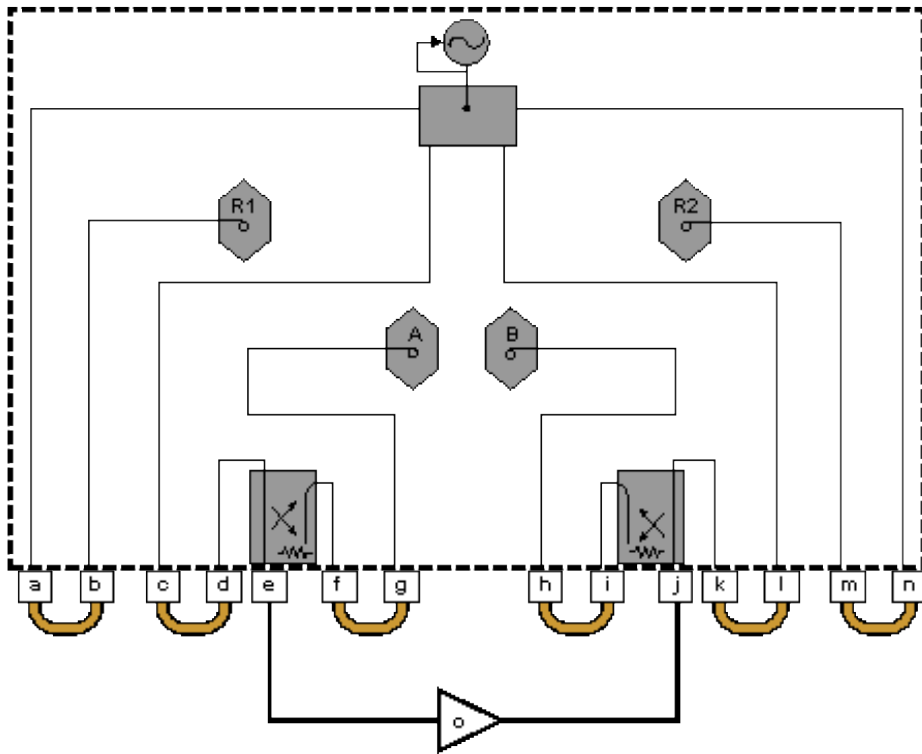

| Item | Description | Item | Description | Item | Description            |
|------|-------------|------|-------------|------|------------------------|
| a    | SOURCE OUT  | h    | RCVR B IN   | o    | DUT, customer supplied |
| b    | RCVR R1 IN  | i    | CPLR ARM    |      |                        |
| c    | SOURCE OUT  | j    | PORT 2      |      |                        |
| d    | CPLR THRU   | k    | CPLR THRU   |      |                        |
| e    | PORT 1      | l    | SOURCE OUT  |      |                        |
| f    | CPLR ARM    | m    | RCVR R2 IN  |      |                        |
| g    | RCVR A IN   | n    | SOURCE OUT  |      |                        |

## Diagram: (E8361A, E8362A/B, E8363A/B, E8364A/B, Option 014) Configuration for High-Power Measurements in the Forward Direction

Explore the graphic with your mouse.

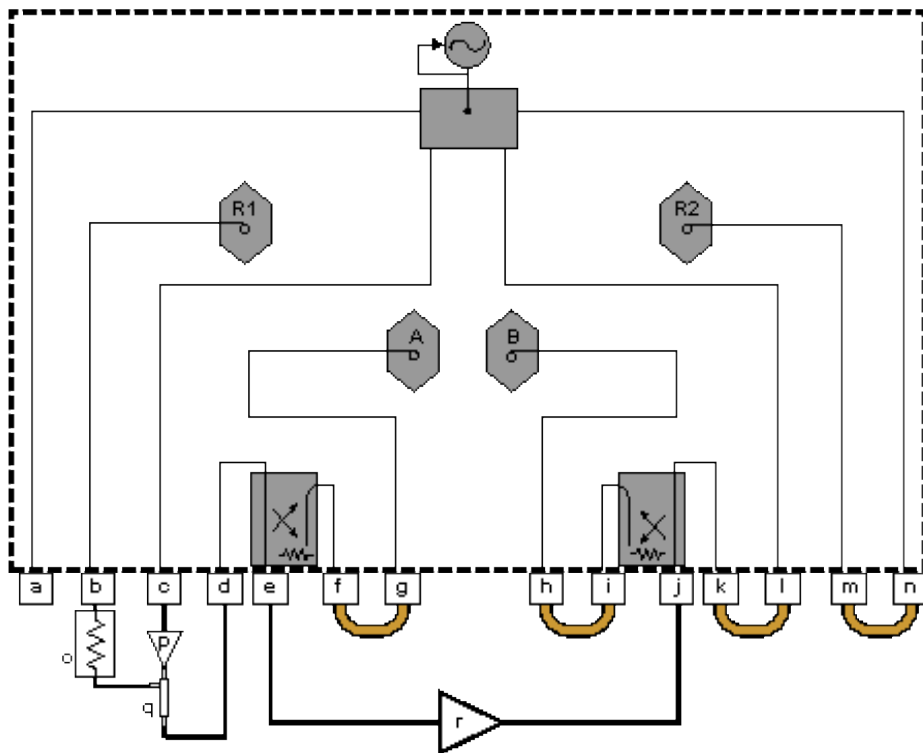


| Item | Description | Item | Description | Item | Description                            |
|------|-------------|------|-------------|------|----------------------------------------|
| a    | SOURCE OUT  | h    | RCVR B IN   | o    | Attenuator, customer supplied          |
| b    | RCVR R1 IN  | i    | CPLR ARM    | p    | Booster amplifier, customer supplied   |
| c    | SOURCE OUT  | j    | PORT 2      | q    | Directional coupler, customer supplied |
| d    | CPLR THRU   | k    | CPLR THRU   | r    | DUT, customer supplied                 |
| e    | PORT 1      | l    | SOURCE OUT  |      |                                        |
| f    | CPLR ARM    | m    | RCVR R2 IN  |      |                                        |
| g    | RCVR A IN   | n    | SOURCE OUT  |      |                                        |

## Diagram: Configuration (with an Isolator) for High-Power Measurements in the Forward Direction

- E8361A, E8362A/B, E8363A/B, E8364A/B, Option 014
- N5230A, Option 225, or 425, or 525
- N5250A

Explore the graphic with your mouse.

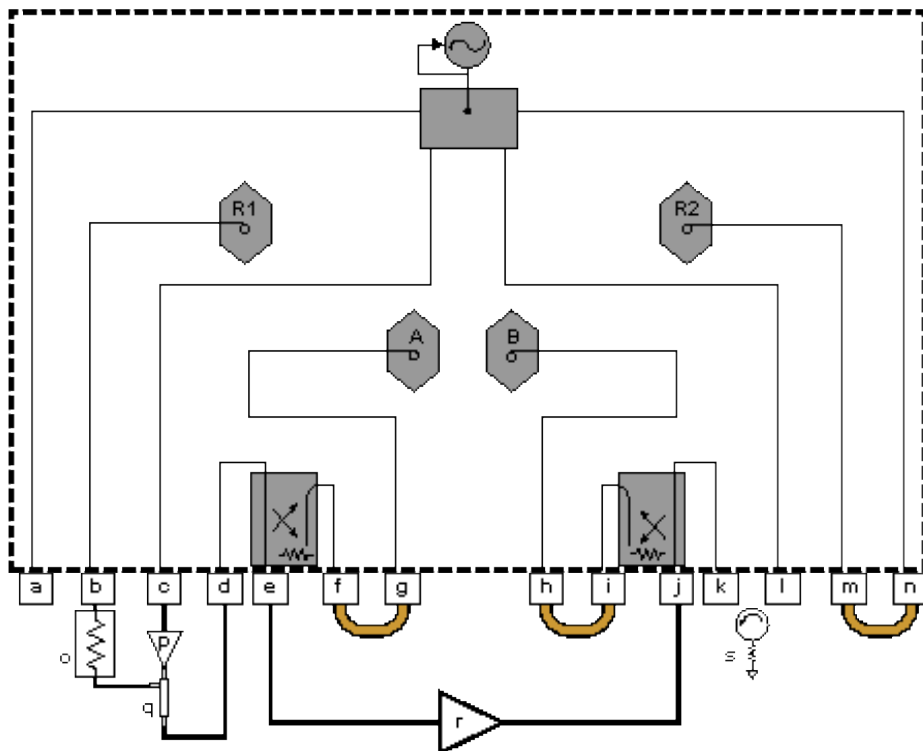

| Item | Description | Item | Description | Item | Description                                                |
|------|-------------|------|-------------|------|------------------------------------------------------------|
| a    | SOURCE OUT  | h    | RCVR B IN   | o    | Attenuator, customer supplied                              |
| b    | RCVR R1 IN  | i    | CPLR ARM    | p    | Booster amplifier, customer supplied                       |
| c    | SOURCE OUT  | j    | PORT 2      | q    | Directional coupler, customer supplied                     |
| d    | CPLR THRU   | k    | CPLR THRU   | r    | DUT, customer supplied                                     |
| e    | PORT 1      | l    | SOURCE OUT  | s    | Isolator, customer supplied (for DUT output above +10 dBm) |
| f    | CPLR ARM    | m    | RCVR R2 IN  |      |                                                            |

**g** RCVR A IN


**n** SOURCE OUT

## Diagram: Configuration using One Booster Amplifier

- E8361A, E8362A/B, E8363A/B, E8364A/B, Option 014
- N5230A, Option 225, or 425, or 525
- N5250A

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains the following components supplied by you: a booster amplifier, a forward coupler, and attenuators.

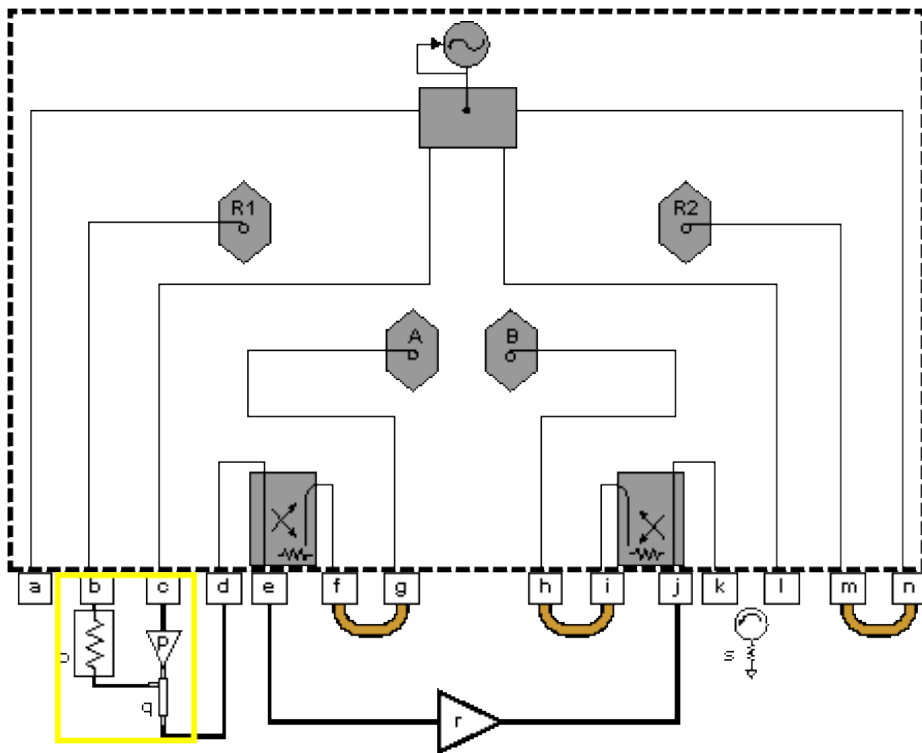



| Item | Description | Item | Description | Item | Description                                                |
|------|-------------|------|-------------|------|------------------------------------------------------------|
| a    | SOURCE OUT  | h    | RCVR B IN   | o    | Attenuator, customer supplied                              |
| b    | RCVR R1 IN  | i    | CPLR ARM    | p    | Booster amplifier, customer supplied                       |
| c    | SOURCE OUT  | j    | PORT 2      | q    | Directional coupler, customer supplied                     |
| d    | CPLR THRU   | k    | CPLR THRU   | r    | DUT, customer supplied                                     |
| e    | PORT 1      | l    | SOURCE OUT  | s    | Isolator, customer supplied (for DUT output above +10 dBm) |
| f    | CPLR ARM    | m    | RCVR R2 IN  |      |                                                            |
| g    | RCVR A IN   | n    | SOURCE OUT  |      |                                                            |




| Item | Description | Item | Description | Item | Description                            |
|------|-------------|------|-------------|------|----------------------------------------|
| a    | SOURCE OUT  | h    | RCVR B IN   | o    | Attenuator, customer supplied          |
| b    | RCVR R1 IN  | i    | CPLR ARM    | p    | Booster amplifier, customer supplied   |
| c    | SOURCE OUT  | j    | PORT 2      | q    | Directional coupler, customer supplied |
| d    | CPLR THRU   | k    | CPLR THRU   | r    | DUT, customer supplied                 |
| e    | PORT 1      | l    | SOURCE OUT  |      |                                        |
| f    | CPLR ARM    | m    | RCVR R2 IN  |      |                                        |
| g    | RCVR A IN   | n    | SOURCE OUT  |      |                                        |

## Diagram: Configuration for High-Power Measurements in both Forward & Reverse Directions

- E8361A, E8362A/B, E8363A/B, E8364A/B, Option 014
- N5230A, Option 225, or 425, or 525
- N5250A


Explore the graphic with your mouse.

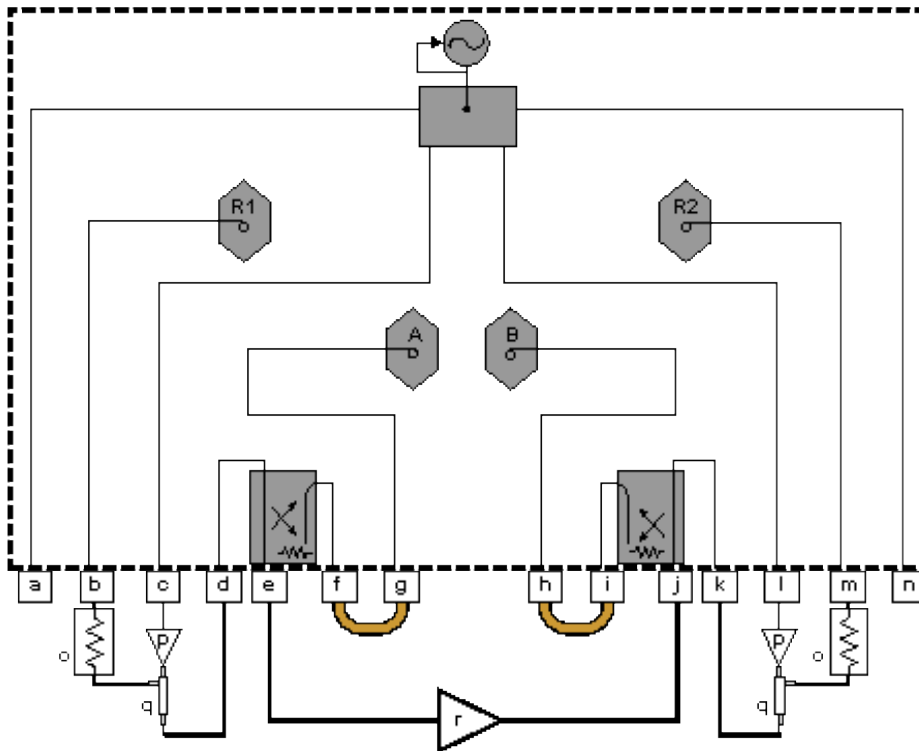

| Item | Description | Item | Description | Item | Description                            |
|------|-------------|------|-------------|------|----------------------------------------|
| a    | SOURCE OUT  | h    | RCVR B IN   | o    | Attenuator, customer supplied          |
| b    | RCVR R1 IN  | i    | CPLR ARM    | p    | Booster amplifier, customer supplied   |
| c    | SOURCE OUT  | j    | PORT 2      | q    | Directional coupler, customer supplied |
| d    | CPLR THRU   | k    | CPLR THRU   | r    | DUT, customer supplied                 |
| e    | PORT 1      | l    | SOURCE OUT  |      |                                        |
| f    | CPLR ARM    | m    | RCVR R2 IN  |      |                                        |
| g    | RCVR A IN   | n    | SOURCE OUT  |      |                                        |




## Diagram: Measuring Calibration Power Levels

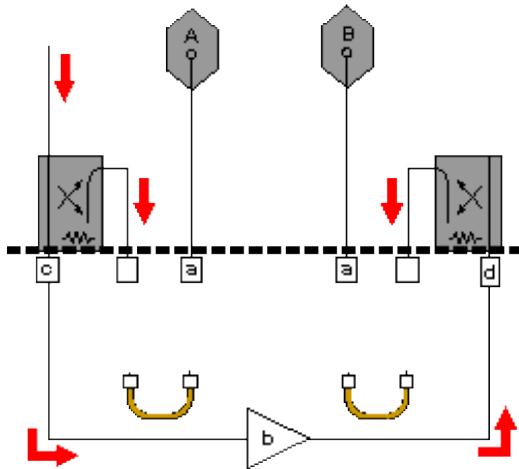

| Item | Description                                                                  |
|------|------------------------------------------------------------------------------|
| a    | Measure the receiver input power where your external circuitry connects here |
| b    | DUT, customer supplied                                                       |
| c    | PORT 1                                                                       |
| d    | PORT 2                                                                       |


## Diagram: (E880xA) Basic Configuration

Explore the graphic with your mouse.

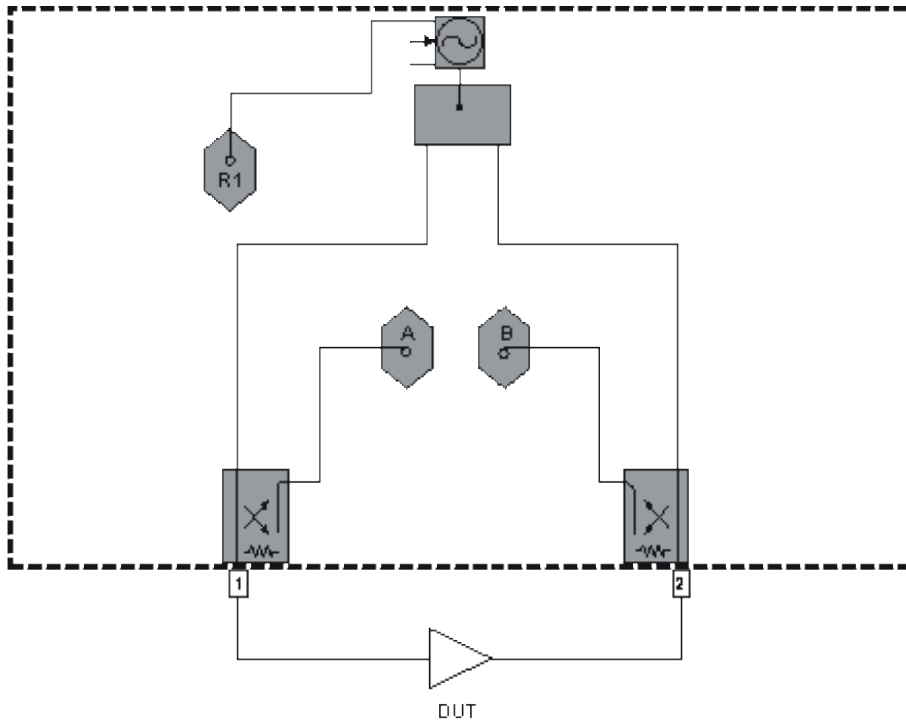

# Diagram: (E880xA) Configuration for High-Power Measurements in the Forward Direction (Single-Port Cal Only)


Explore the graphic with your mouse.

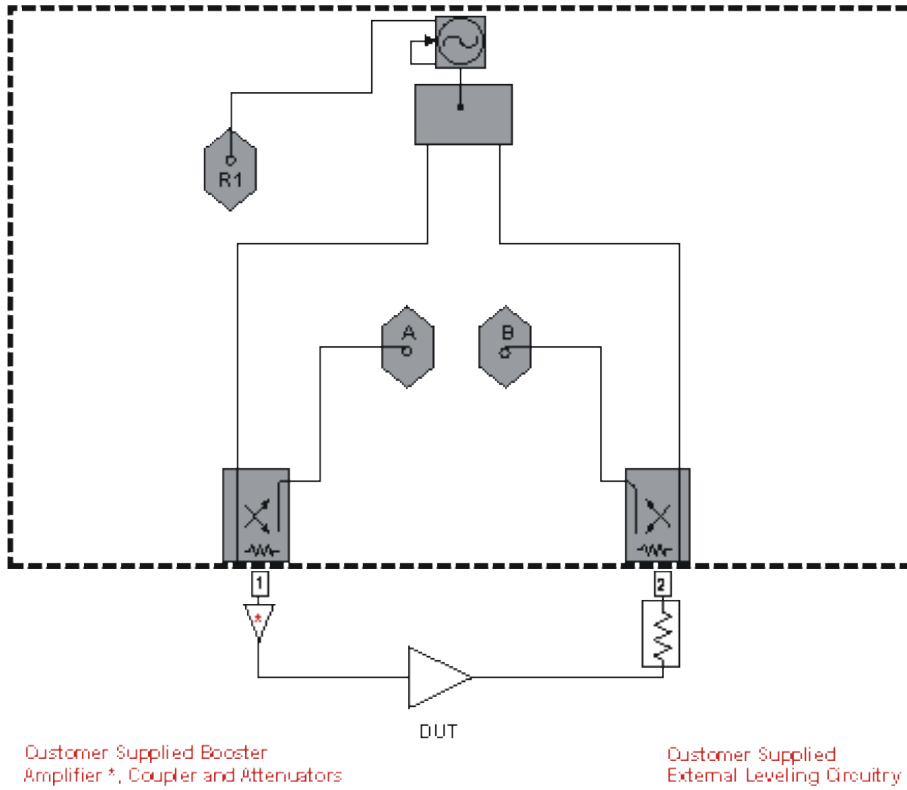



## Diagram: (E880xA) Configuration for Non-Boosted High-Power Measurements in both Forward and Reverse Directions

Explore the graphic with your mouse.

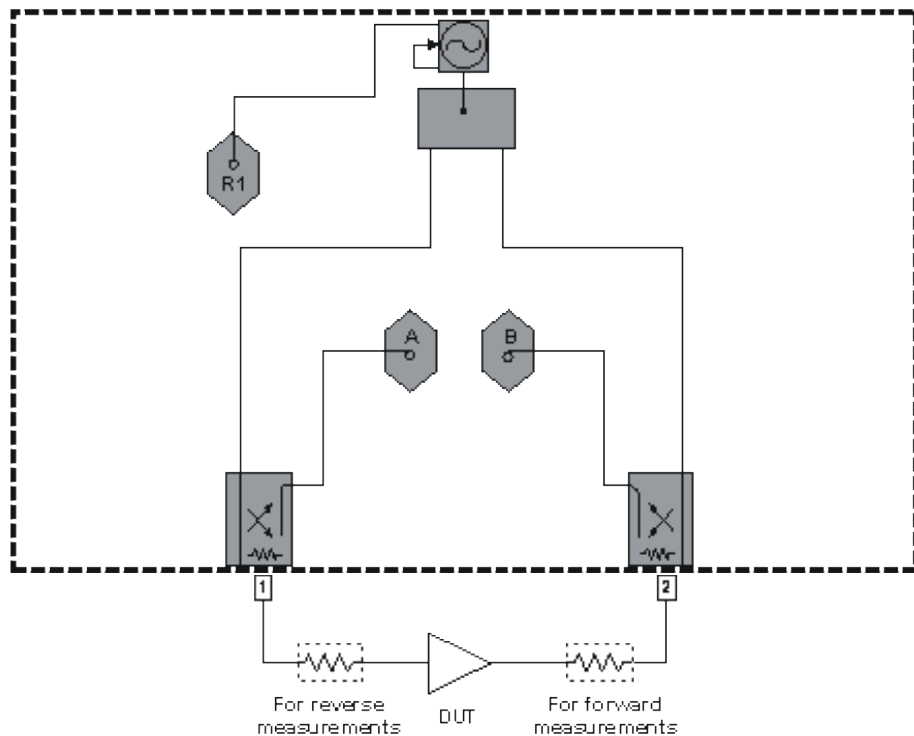


Customer Supplied Attenuator - Location  
Dependent on Direction of Measurement

## Diagram: (E880xA) Configuration using a Booster Amp

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains a booster amplifier supplied by you.

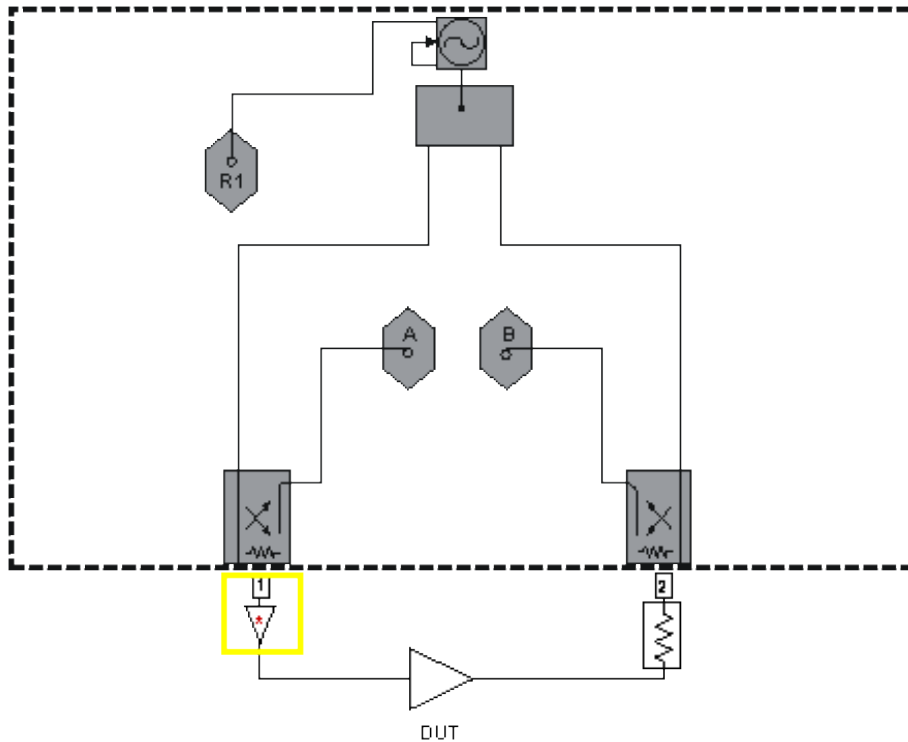


Customer Supplied Booster  
Amplifier \*, Coupler and Attenuator

Customer Supplied  
External Leveling Circuitry

## Diagram: (E880xA) External Leveling Configuration

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, forward coupler, attenuator, and negative detector diode.

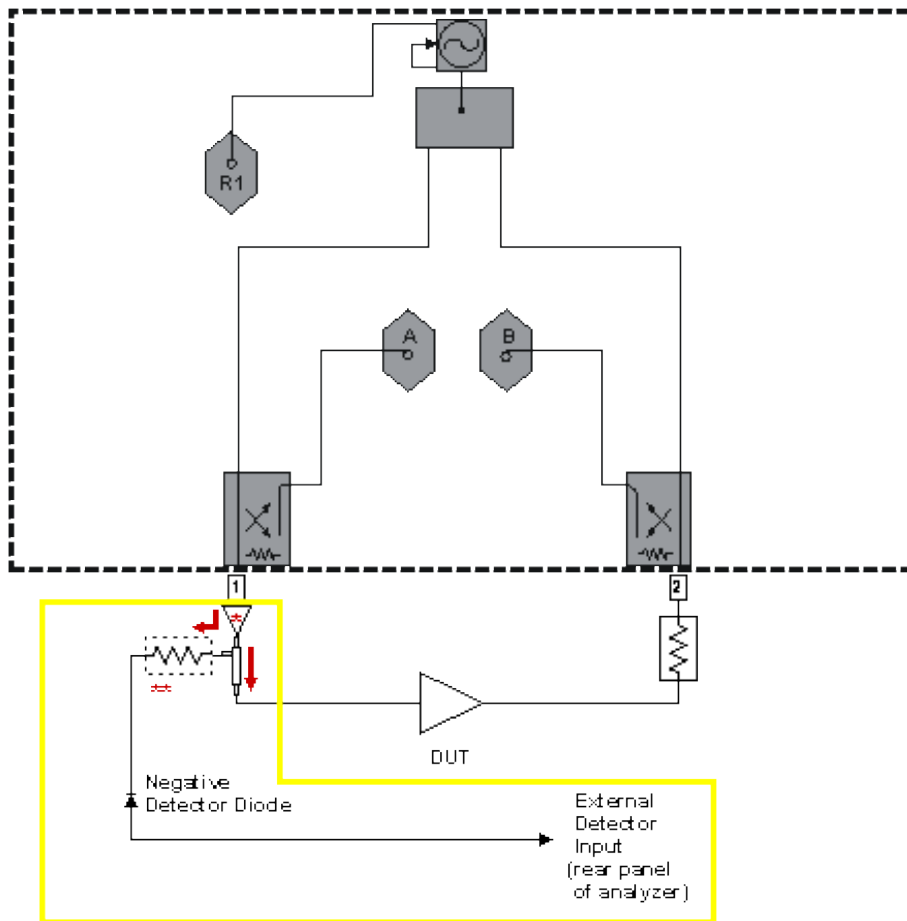


Customer Supplied Booster Amplifier <sup>\*</sup>,  
Negative Detector Diode, Coupler and Attenuators

<sup>\*\*</sup> This attenuator may be required to meet  
the recommended power level input  
( +10dBm to -20dBm ) of the detector diode.


# Diagram: (E880xA, Option 014) Basic Configuration

Explore the graphic with your mouse.

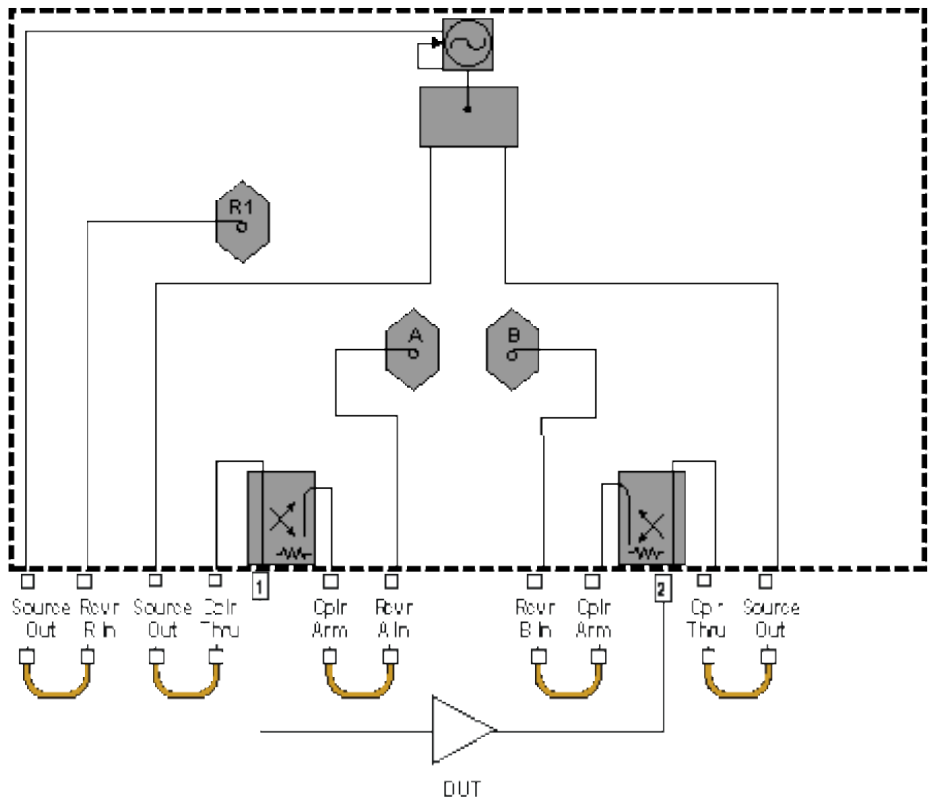

# Diagram: (E880xA, Option 014) Configuration for High-Power Measurements in the Forward Direction

Explore the graphic with your mouse.

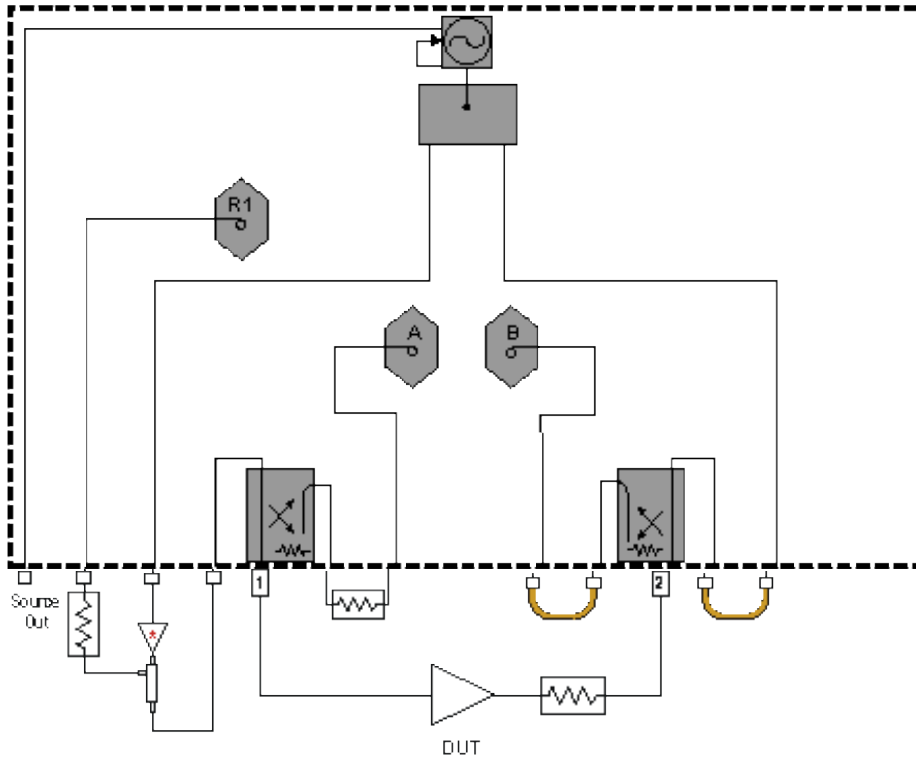


Customer Supplied Booster  
Amplifier \*, Coupler, and Attenuators



# Diagram: (E880xA, Option 014) Configuration for High-Power Measurements in both Forward and Reverse Directions

Explore the graphic with your mouse.

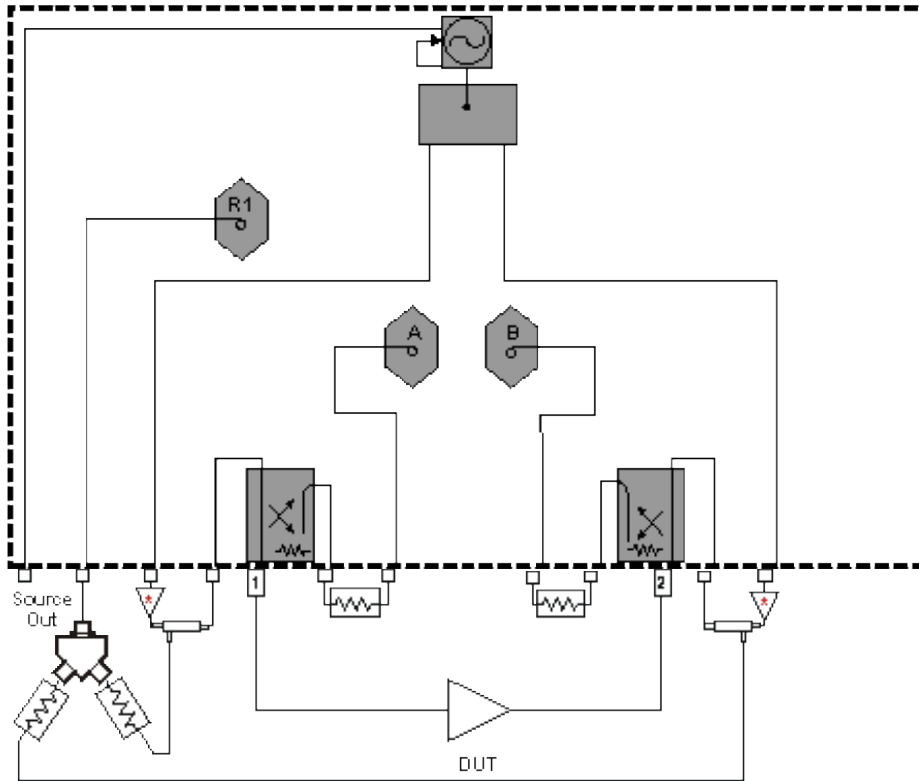

Customer Supplied Booster Amplifiers \*,  
Couplers, Attenuators and Power Splitter






## Diagram: (E880xA, Option 014) Configuration Using Two Booster Amplifiers

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains the following components supplied by you - two booster amplifiers, two forward couplers, two attenuators, and a power splitter.

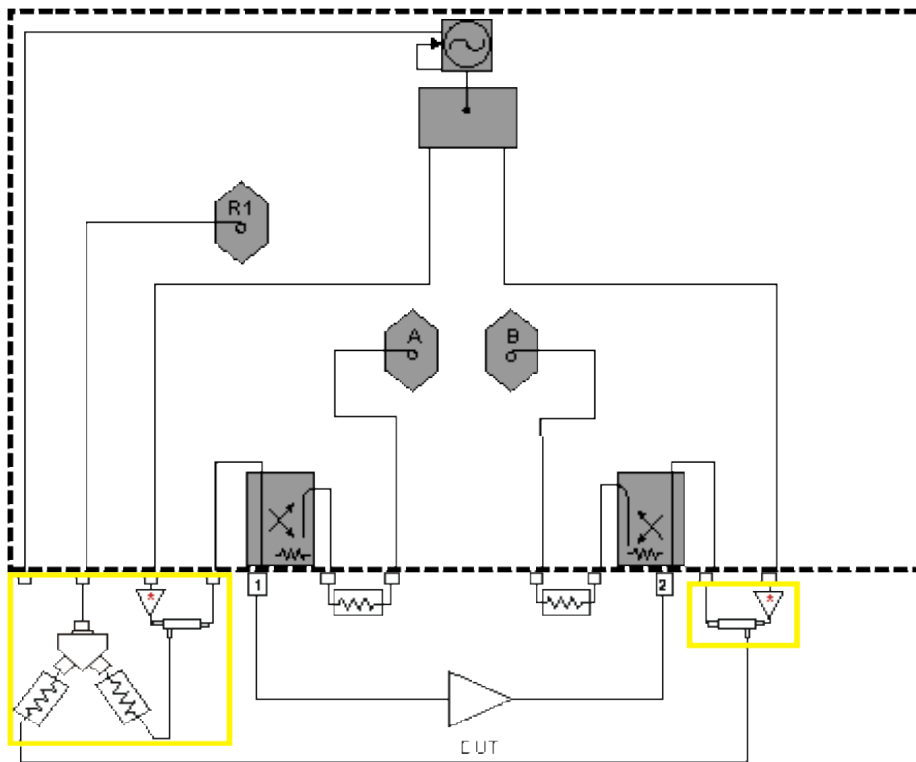


Customer Supplied Booster Amplifiers ^,  
Couplers, Attenuators and Power Splitter

## Diagram: (E880xA, Option 014) External Leveling using One Booster Amplifier

Explore the graphic with your mouse.


**Note:** the circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, a forward coupler, two attenuators, a power splitter, and a negative detector diode.

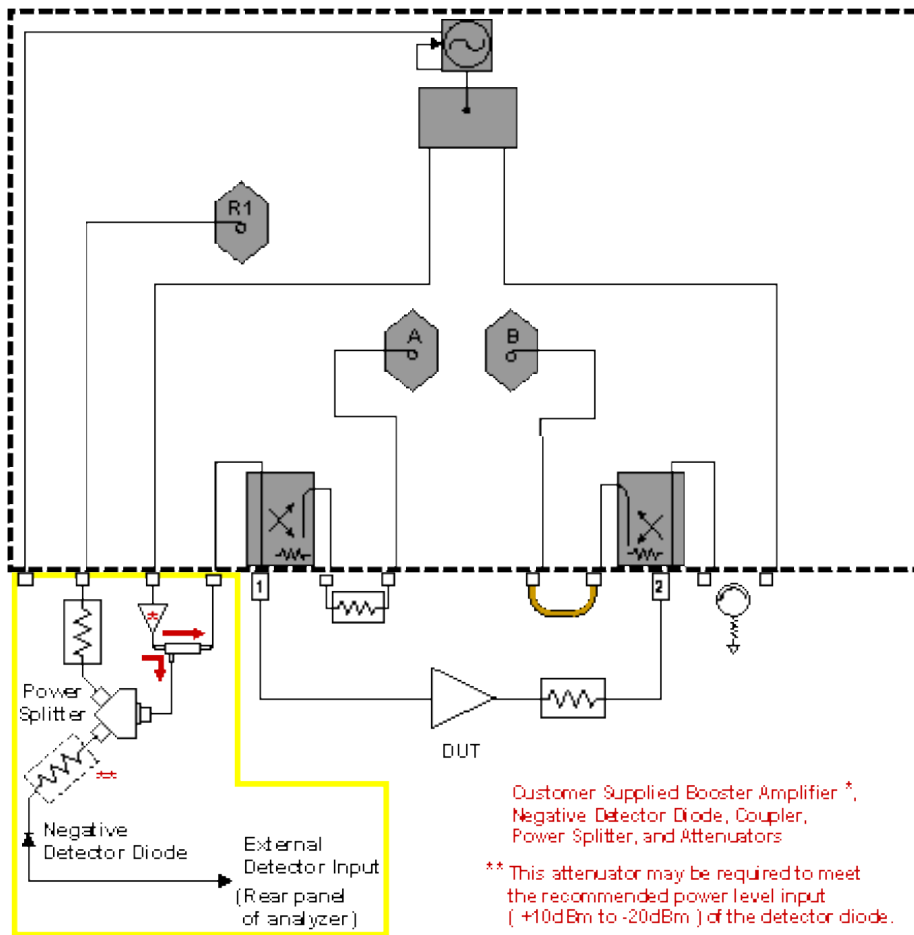

## Diagram: (E880xA, Option 014) External Leveling using Two Booster Amplifiers

Explore the graphic with your mouse.


**Note:** the circuitry inside the yellow lines contains the following components supplied by you - two booster amplifiers, two forward couplers, two attenuators, four power splitters, and a negative detector diode.

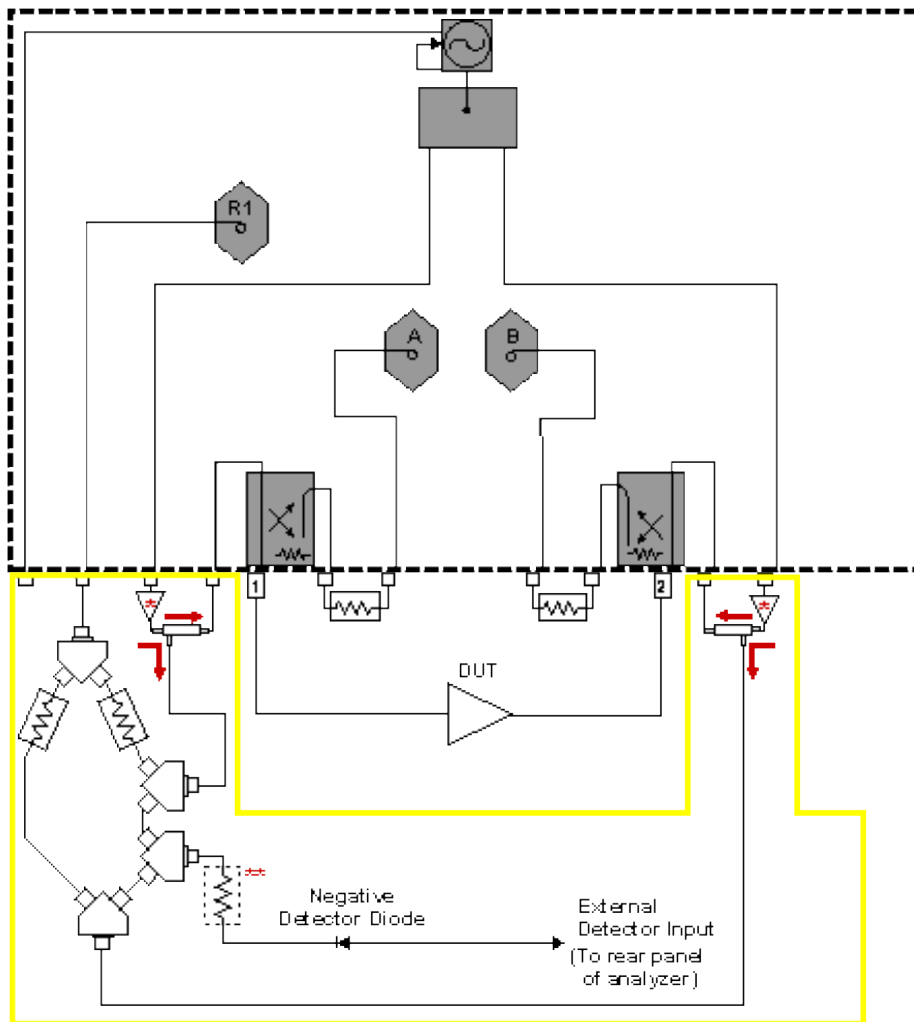

\*\* This attenuator may be required to meet the recommended power level input ( +10dBm to -20dBm ) of the detector diode.

Customer Supplied Booster Amplifiers \*\*, Couplers, Negative Detector Diode, Attenuators and Power Splitters

## Diagram: (E880xA, Option 014) Measuring Calibration Power Levels

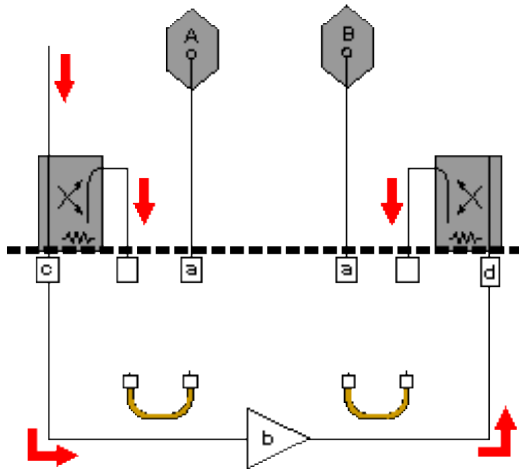


| Item | Description |
|------|-------------|
|------|-------------|

- |   |                                                                              |
|---|------------------------------------------------------------------------------|
| a | Measure the receiver input power where your external circuitry connects here |
| b | DUT, customer supplied                                                       |
| c | PORT 1                                                                       |
| d | PORT 2                                                                       |

## Diagram: (N338x) Basic Configuration

Explore the graphic with your mouse.


**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT.

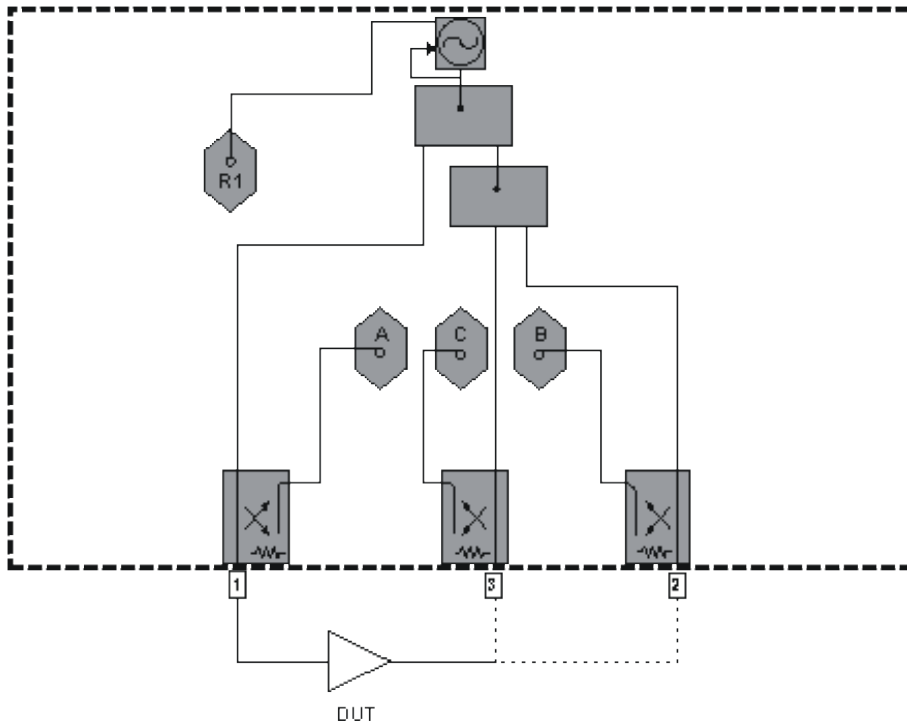

# Diagram: (N338x) Configuration for High-Power Measurements in the Forward Direction (Single-Port Cal Only)

Explore the graphic with your mouse.


**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT.

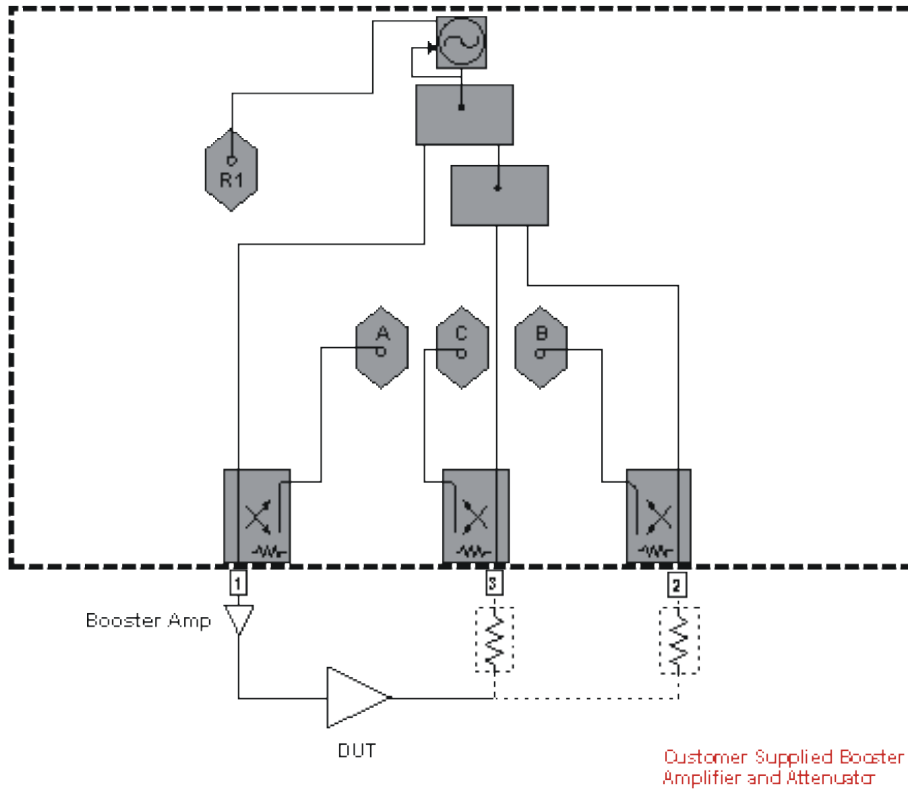

## Diagram: (N338x) Configuration for Non-Boosted High-Power Measurements in both Forward and Reverse Directions

Explore the graphic with your mouse.


**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT.

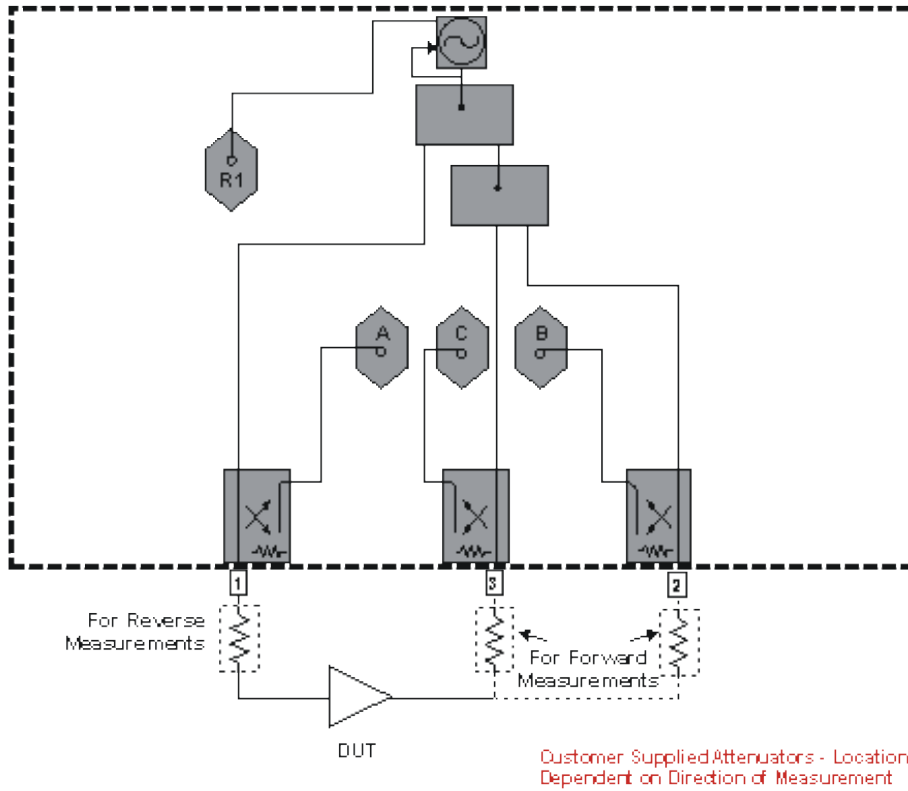

## Diagram: (N338x) Configuration using a Booster Amplifier

Explore the graphic with your mouse.

**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT. The circuitry inside the yellow lines contains a booster amplifier supplied by you.

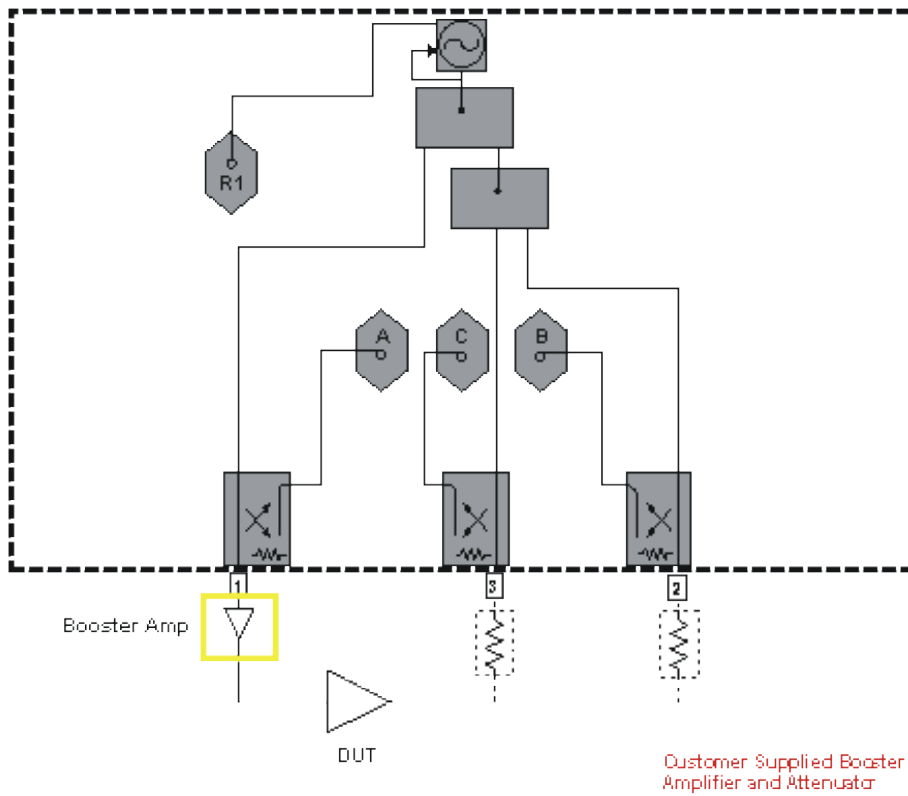




## Diagram: (N338x) External Leveling Configuration

Explore the graphic with your mouse.

**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT. The circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, a forward coupler, an attenuator, and a negative detector diode.

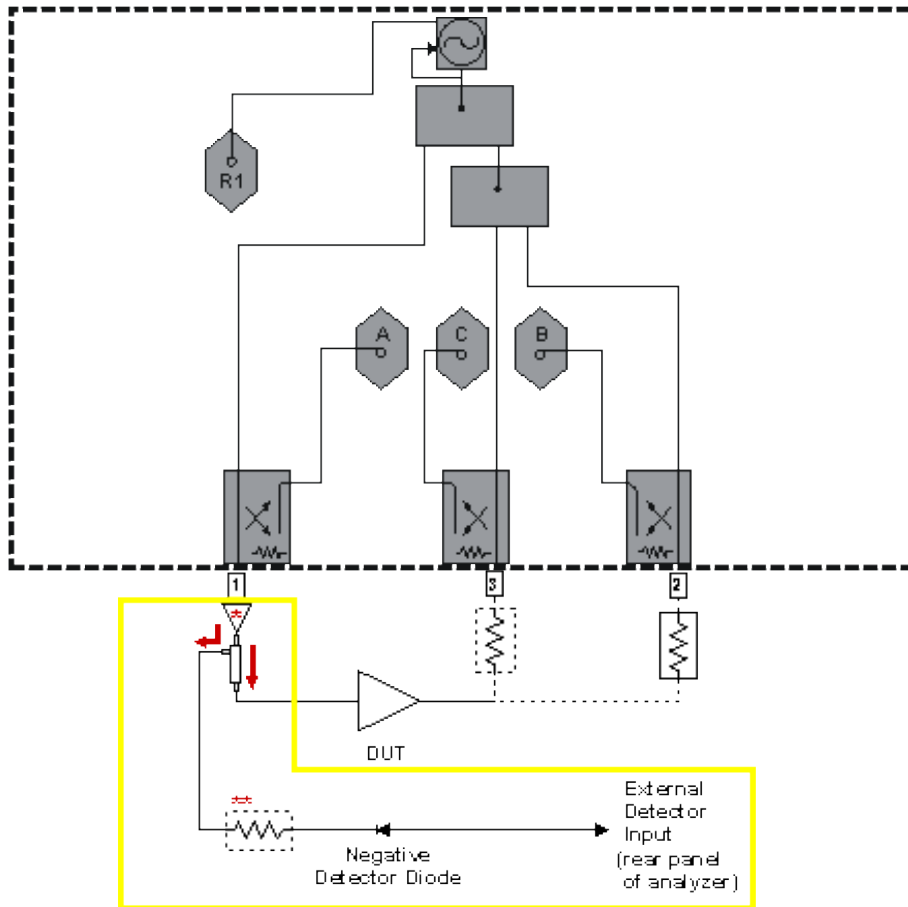


Customer Supplied Booster Amplifier \*,  
Negative Detector Diode, Coupler and Attenuators

\*\* This attenuator may be required to meet  
the recommended power level input  
( +10dBm to -20dBm ) of the detector diode.

## Diagram: (N338xA, Option 014) Basic Configuration


Explore the graphic with your mouse.

**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT.

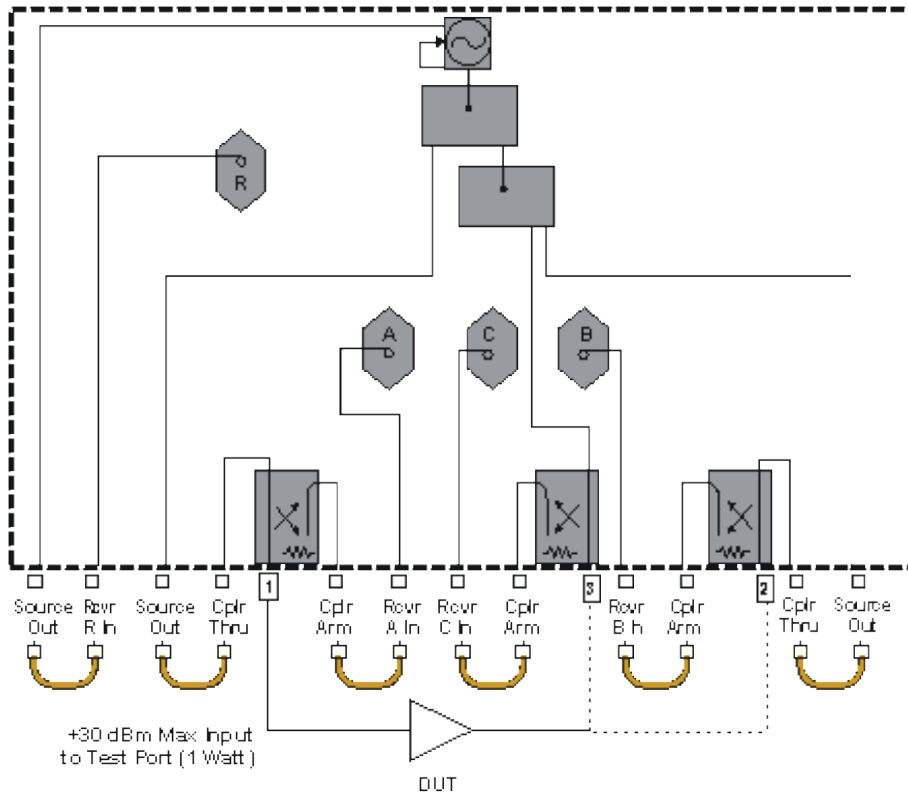


# Diagram: (N338xA, Option 014) Configuration for High-Power Measurements in the Forward Direction

Explore the graphic with your mouse.

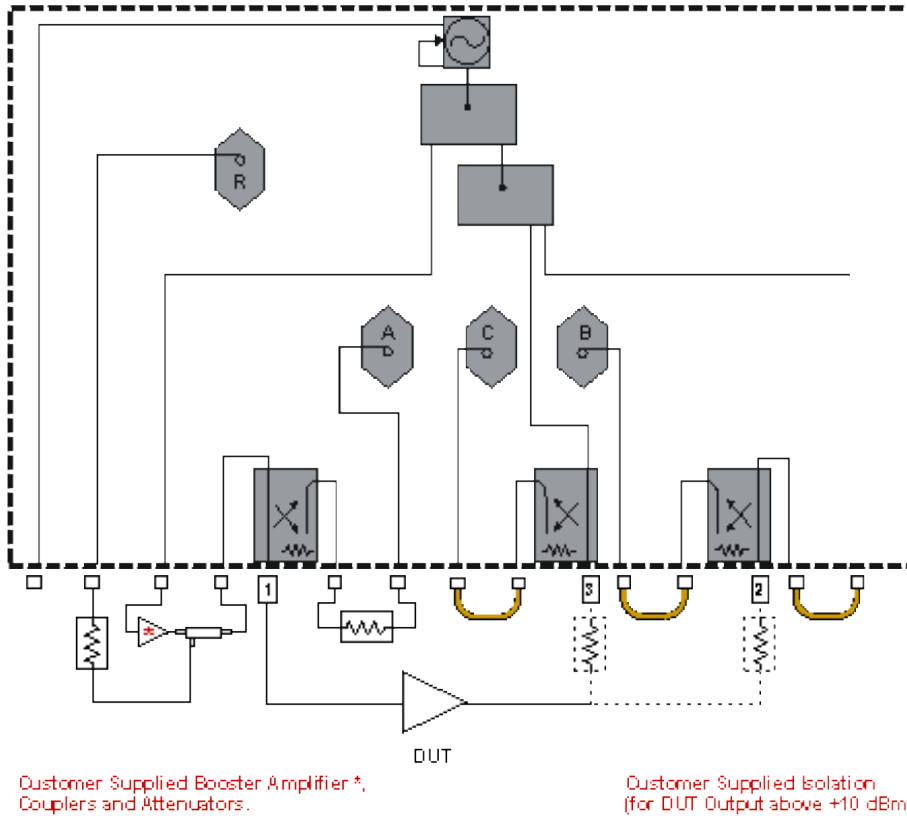


# Diagram: (N338xA, Option 014) Configuration (with an Isolator) for High-Power Measurements in the Forward Direction

Explore the graphic with your mouse.

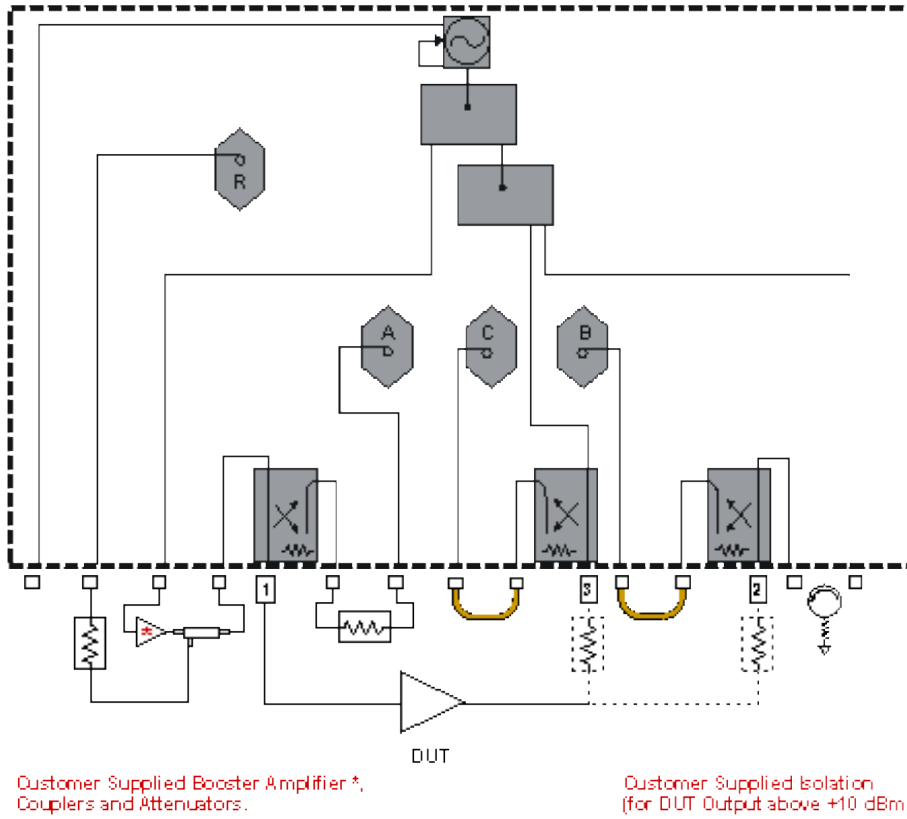

# Diagram: (N338xA, Option 014) Configuration for High-Power Measurements in both Forward and Reverse Directions

Explore the graphic with your mouse.

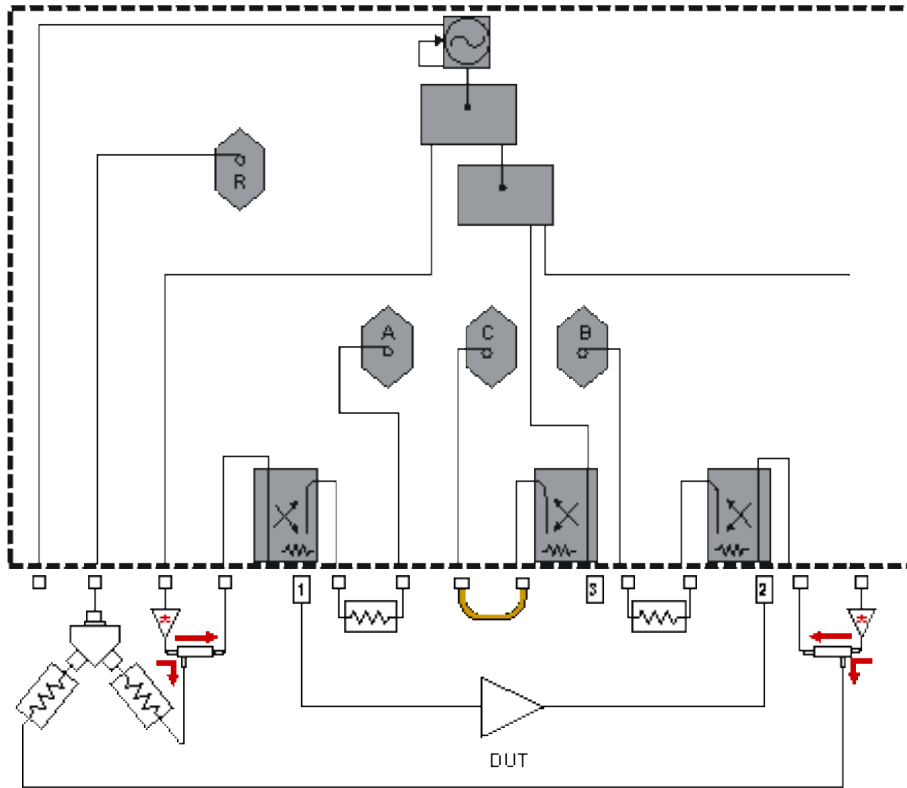


Customer Supplied Booster Amplifiers \*,  
Couplers, Attenuators and Power Splitter

## Diagram: (N338xA, Option 014) Configuration Using One Booster Amplifier

Explore the graphic with your mouse.

**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT. The circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, a forward coupler, and an attenuator.

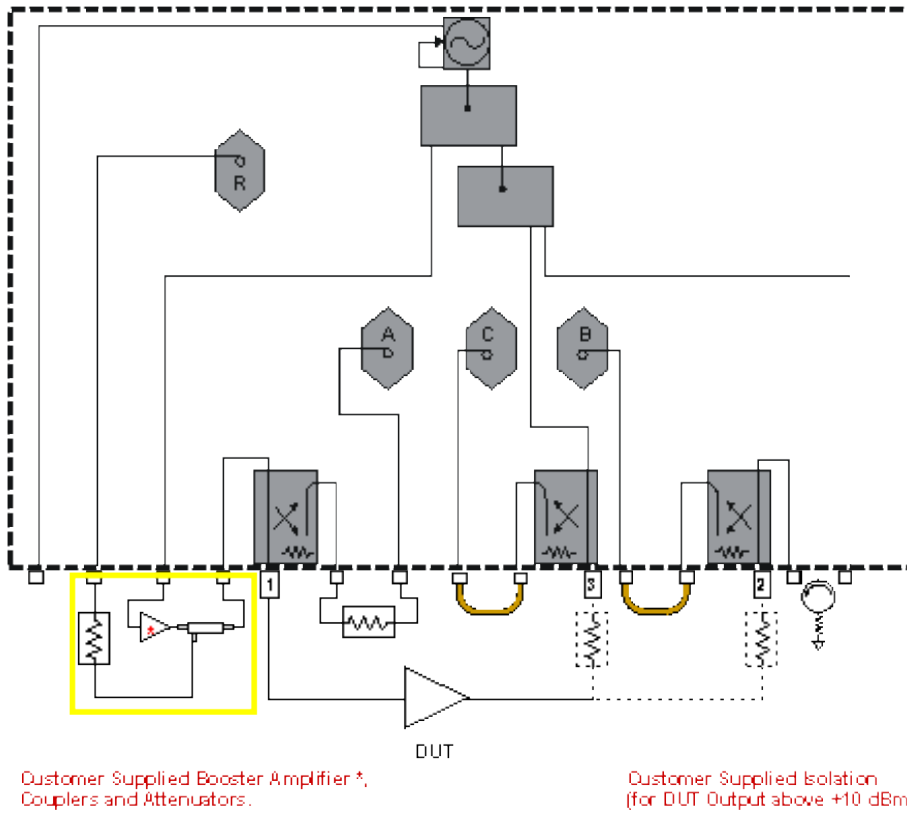




## Diagram: (N338xA, Option 014) External Leveling using One Booster Amplifier

Explore the graphic with your mouse.

**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT. The circuitry inside the yellow lines contains the following components supplied by you - a booster amplifier, a forward coupler, two attenuators, a power splitter and a negative detector diode.

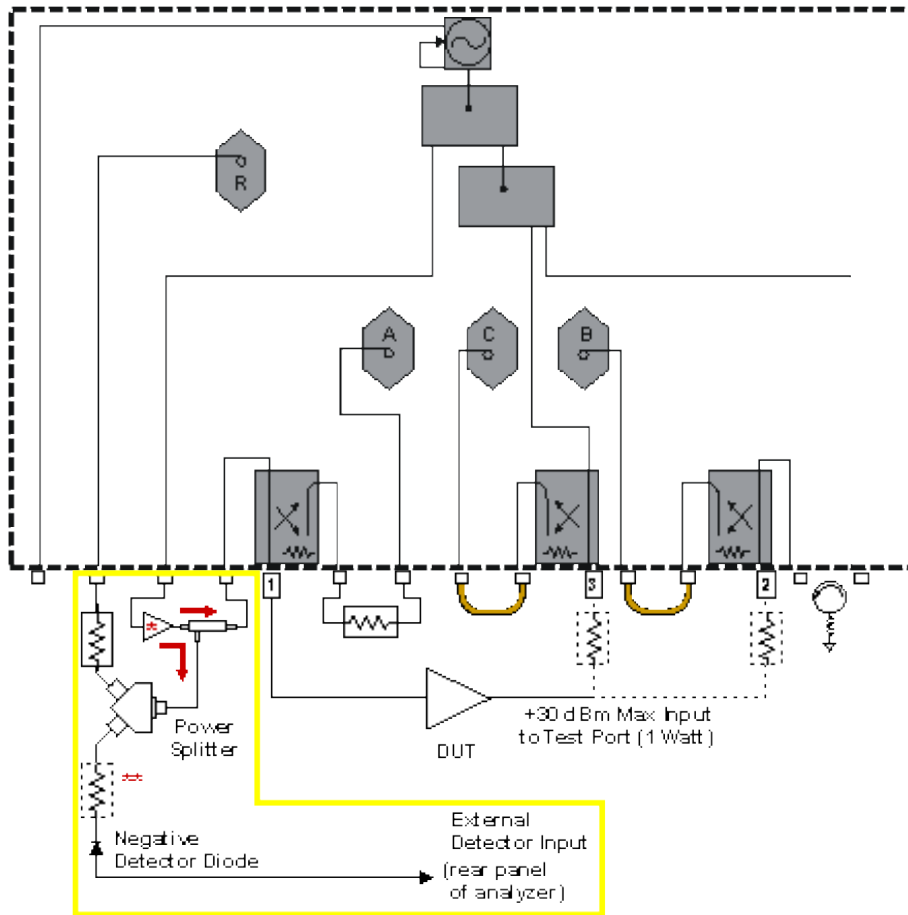

Customer Supplied Booster Amplifier \*,  
Negative Detector Diode, Couplers and Attenuators.


Customer Supplied Isolation  
(for DUT Output above +10 dBm)



## Diagram: (N338xA, Option 014) External Leveling using Two Booster Amplifiers

Explore the graphic with your mouse.

**Note:** the circuitry inside the yellow lines contains the following components supplied by you - two booster amplifiers, two forward couplers, two attenuators, three power splitters, and a negative detector diode.

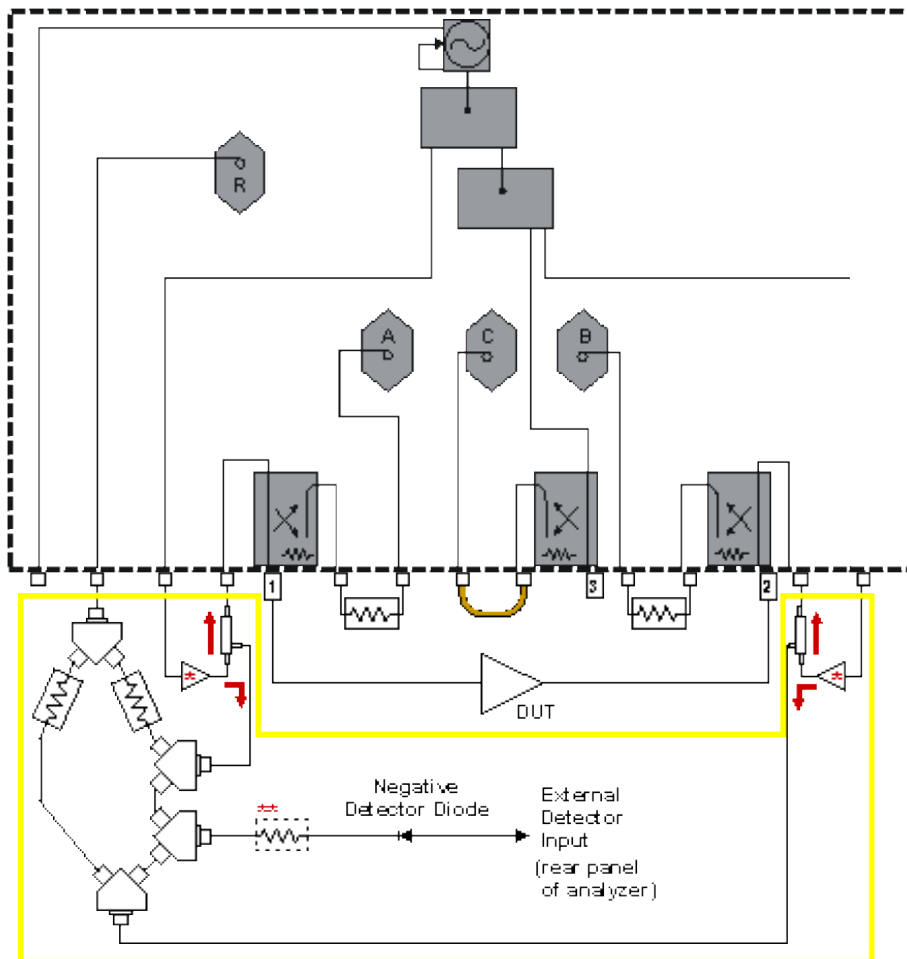


Customer Supplied Booster Amplifier \*,  
Negative Detector Diode, Coupler,  
Power Splitter, and Attenuators

\*\* This attenuator may be required to meet  
the recommended power level input  
( +10dBm to -20dBm ) of the detector diode.

## Diagram: (N338xA, Option 014) Measuring Calibration Power Levels

**Note:** Either Port 2 or Port 3 can be used for testing a 2-Port DUT.

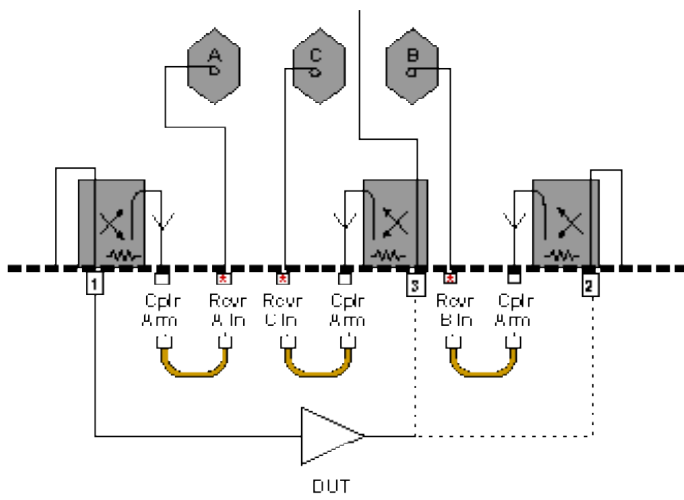

\* Measure the receiver input power where your external circuitry connects here.

## Easy versus Secure Configuration

---

When upgrading Firmware on the PNA, you encounter a **Choose Configuration** dialog box. This is used to determine the level of security set for the DCOM interface on the PNA. For more detailed information on the security settings for the DCOM interface, including a procedure for making these settings manually, see [Configure for COM-DCOM Programming](#).

Comparison of the "Easy and More Secure" settings are as follows:

### Easy Connection:

- No configuration of the PNA required for remote access to connect.
- Anyone on the local subnet can access the PNA remotely.
- People from other NT domains can connect to the PNA.

### More Secure:

- Requires creating users on the PNA or adding the PNA to a domain
- An administrator of the PNA can specify users or groups that are allowed remote access to the PNA application

## Changing Network Client

---

If your PC network uses Novell NetWare servers, a change must be made to the PNA setup before it can operate on your network. If you are unsure, ask your local IT department.

---

**Note:** Do NOT **Uninstall** "Client for Microsoft Networks". This will prevent proper operation of the PNA..

---

To remove "Client for Microsoft Networks" (Remove is different from Uninstall):

1. From the PNA Desktop, right-click **My Network Places**
2. Click **Properties**
3. Right-click **Local Area Connection**
4. Click **Properties**
5. Click (remove the check from) **Client for Microsoft Networks**

To install "Client Service for NetWare".

1. Click **Install**
2. In **Select Network Component Type**, make sure **Client** is selected
3. Click **Add**
4. In **Select Network Client**, make sure **Client Service for NetWare** is selected
5. Click **OK**.

## Troubleshooting the PNA

---

By running a few checks, you can identify if the analyzer is at fault. Before calling Agilent Technologies or returning the instrument for service, please make the following checks.

### [Check the Basics](#)

### [PNA Application Terminates Unexpectedly](#)


### [Check Error Terms](#)

### [Check the Service Guide](#)

## **Other Support Topics**

### **Check the Basics**

A problem can often be solved by repeating the procedure you were following when the problem occurred. Before calling Agilent Technologies or returning the instrument for service, please make the following checks:

1. Is there power at the power socket? Is the instrument plugged in?
2. Is the instrument turned on? Check to see if the front panel line switch and at least one of the LED rings around the test ports glows green. This indicates the power supply is on.
3. If you are experiencing difficulty with the front-panel keypad or peripherals, the USB bus may be overloaded. Remove the USB devices, restart the PNA, and reconnect the USB devices. See [Power-up](#).
4. If other equipment, cables, and connectors are being used with the instrument, make sure they are connected properly and operating correctly.
5. Review the procedure for the measurement being performed when the problem appeared. Are all the settings correct?
6. If the instrument is not functioning as expected, return the unit to a known state by pressing the **Preset** key.
-  7. Is the measurement being performed, and the results that are expected, within the [specifications](#) and capabilities of the instrument?
8. If the problem is thought to be due to firmware, check to see if the instrument has the [latest firmware](#) before starting the troubleshooting procedure.
9. Check that the measurement calibration is valid. See [Accurate Measurement Calibrations](#) for more information.
10. If the necessary test equipment is available, perform the operator's check and system verification in Chapter 2 of the PNA Service Guide, "System Tests, Verifications, and Adjustments," . You can download a copy of the Service Guide from our Web site: <http://www.agilent.com>.


### **PNA Application Terminates Unexpectedly**

If an unexpected and irrecoverable error occurs, Agilent would like to know about it. The PNA attempts to save pertinent information about the state of the system. **The PNA does NOT send this information to Agilent.**

We respect the privacy of our customers. However, access to information that helps us improve the PNA is a benefit to both Agilent and you. Please take the time to contact us or email the saved information to [na\\_support@agilent.com](mailto:na_support@agilent.com).

The following procedure shows how to do this:

1. A message box immediately appears on the screen containing the location of a directory. Please record this message. If you miss the message, you can find the directory location using the Windows Event Log: On the PNA, click Start, Settings, Control Panel, Administrative Tools, Event Viewer. Double-click the top line (most recent event). The location of the directory is seen in the Description.
2. A dialog box may appear on the screen (shown below) allowing you to add comments to help us replicate the crash.
3. Find the directory (described in Step 1) which contains the following files:
  - 835x.dmp which is the 835x.exe capturing the context in which the program crashed.
  - 835x.xml which reports some very basic information ( exception code, OS version, and the list of modules loaded at the time of the crash and their respective version numbers).
  - 835xCrashLog.txt: The text file with your comments (described in Step 2), if submitted.
4. If your PNA is not connected to LAN or is not configured to send email, copy the files to a PC. Then, please email the files to [na\\_support@agilent.com](mailto:na_support@agilent.com)

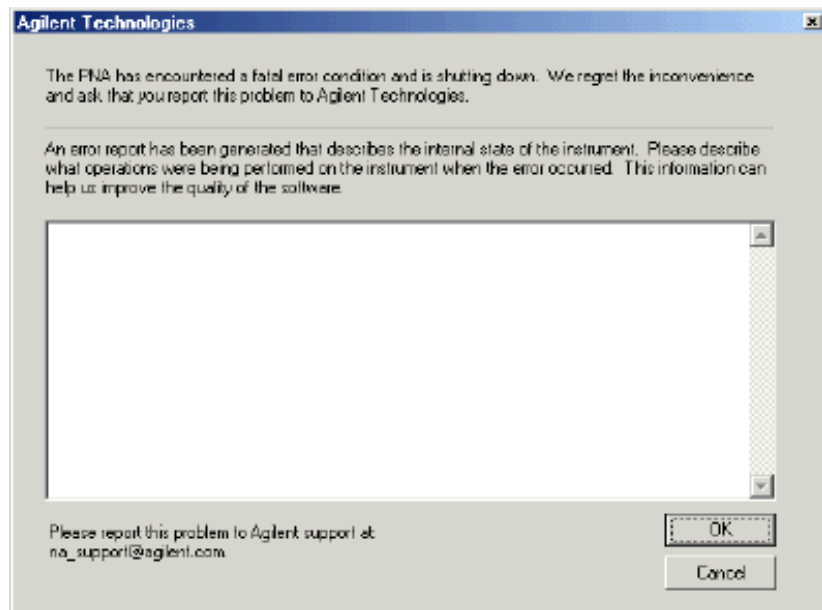

## Check Error Terms

If you print the error terms at set intervals (weekly, monthly, and so forth), you can compare current error terms to these records. A stable, repeatable system should generate repeatable error terms over long time intervals, for example, six months. If a subtle failure or mild performance problem is suspected, the magnitude of the error terms should be compared against values generated previously with the same instrument and calibration kit. See the [procedure for monitoring error terms](#).

- A long-term trend often reflects drift, connector and cable wear, or gradual degradation, indicating the need

for further investigation and preventative maintenance. Yet, the system may still conform to specifications. The cure is often as simple as cleaning and gaging connectors or inspecting cables.

- A sudden shift in error terms reflects a sudden shift in systematic errors, and may indicate the need for further troubleshooting.

Consider the following while troubleshooting:

- All parts of the system, including cables and calibration devices, can contribute to systematic errors and impact the error terms.
- Connectors must be clean and gauged, and within specification for error term analysis to be meaningful. See the Chapter 2 in the PNA Service Guide for information on cleaning and gaging connectors.
  - Avoid unnecessary bending and flexing of the cables following measurement calibration, thus minimizing cable instability errors.
  - Use good connection techniques during the measurement calibration. The connector interface must be repeatable. See the PNA Service Guide for information on connection techniques.
- It is often worthwhile to perform the procedure twice (using two distinct measurement calibrations) to establish the degree of repeatability. If the results do not seem repeatable, check all connectors and cables.
- Use error-term analysis to troubleshoot minor, subtle performance problems. See Chapter 3, "Troubleshooting," in the PNA Service Guide if a blatant failure or gross measurement error is evident.

## **Check the Service Guide**

Check the PNA Service Guide for specific troubleshooting procedures to help identify problems. You can download a copy of the Service Guide from our Web site: <http://www.agilent.com>.

## PNA Error Messages

---

[500 - 750 Calibrate](#)

[770 - 1000 Hardware](#)

[1000 - 1200 Measure](#)

[1281 - 1535 Parser](#)

[1536 - 1650 Display](#)

[1700 - 2000 Channel](#)

[2048 - 2200 General](#)

[Standard SCPI Errors](#)

---

**Note:** The **EventID**'s listed below are provided for COM programming. For more information, see [Working with PNA Events](#)

---

For more information on PNA error messages ([see Error Messages](#)).

---

### Cal Errors

---

#### Message: 512

"A secondary parameter (power, IFBW, sweeptime, step mode) of the calibrated state has changed."


**Severity:** Informational

**Further explanation:** The calibration is questionable when any of these secondary parameters change after the calibration is performed.

**Suggestions:** If you require an accurate measurement with the new settings, repeat the calibration.

**EventID:** 68020200 (hex)

#### Message: 513

 Calibration cannot be completed until you have measured all the necessary standards for your selected Cal Type."

**Severity:** Informational

**Further explanation:** You probably received this message because you attempted to turn correction on without first measuring all of the calibration standards

**Suggestions:** Finish measuring the cal standards

**EventID:** 68020201 (hex)

#### Message: 514

"Calibration set has been recalled using a file previously saved on an analyzer that had a different hardware configuration."

**Severity:** Informational

**Further explanation:**

**Suggestions:**

**EventID:** 68020202 (hex)



**Message: 515**

"Calibration is required before correction can be turned on. Channel number is <x>, Measurement is <x>."

**Severity:** Informational

**Further explanation:** There are no error correction terms to apply for the specified channel and measurement.

**Suggestions:** Perform or recall a calibration

**EventID:** 68020203 (hex)

**Message: 516**

"Critical parameters in your current instrument state do not match the parameters for the calibration set, therefore correction has been turned off. The critical instrument state parameters are sweep type, start frequency, frequency span, and number of points."

**Severity:** Informational

**Further explanation:** None

**Suggestions:** You can either recalibrate using the new settings or change back to the original setting that was used when the calibration was performed.

**EventID:** 68020204 (hex)

**Message: 517**

"Interpolation is turned off and you have changed the stimulus settings of the original calibration, so correction has been turned off."

**Severity:** Informational

**Further explanation:** The most accurate calibration is maintained only when the original stimulus settings are used.

**Suggestions:** If reduced accuracy is OK, set interpolation ON to allow stimulus setting changes.

**EventID:** 68020205 (hex)

**Message: 518**

"Interpolation is turned off and you have selected correction ON. Correction has been restored with the previous stimulus settings."

**Severity:** Informational

**Further explanation:** None

**Suggestions:** None

**EventID:** 68020206 (hex)

**Message: 519**

"Stimulus settings for your current instrument state exceeded the parameters of the original calibration, so correction has been turned off."

**Severity:** Informational

**Further explanation:** Correction data outside the stimulus settings does not exist.

**Suggestions:** Perform a broadband calibration, with increased numbers of points with interpolation ON, to maintain calibration over the widest possible stimulus frequency settings.

**EventID:** 68020207(hex)

**Message: 520**

"Cal Type is set to NONE for Channel <x>, Measurement <x>; please select Calibration menu or press Cal hard key."

**Severity:** Informational

**Further explanation:** A cal operation can not proceed until a calibration exists or the cal type is selected. This error can occur if the calibration can not be found. Also this error can happen if a calibration type is not specified before attempting to programmatically execute cal acquisitions.

**Suggestions** To find a calibration, select a Cal Set that contains the calibration needed for the current measurements. OR specify the cal type before beginning a calibration procedure.

**EventID:** 68020208 (hex)

**Message: 521**

"The measurement you set up does not have a corresponding calibration type, so correction has been turned off or is not permitted."

**Severity:** Informational

**Further explanation:** The calibration for the channel may apply only to certain S-Parameters. For example, a 1-Port calibration for S11 can not be applied to a 1-Port calibration applied to S22.

**Suggestions:** Select a calibration type, such as full 2-Port cal, that can be applied to all the measurements to be selected.

**EventID:** 68020209 (hex)

**Message: 522**

"The calibration type you selected cannot be set up."

**Severity:** Informational

**Further explanation:** "Please use the SCPI command ROUTe:PATH:DEFine:PORT <num>,<num> for full 2 port type port assignment."

**Suggestions:**

**EventID:** 6802020A (hex)

**Message: 523**

"The calibration path you selected cannot be set up because it is not valid for the current measurement."

**Severity:** Informational

**Further explanation:** "Please use the SCPI command ROUTe:PATH:DEFine:PORT <num>,<num> for full 2 port type port assignment related to your current measurement."

**Suggestions:**

**EventID:** 6802020B (hex)

**Message: 524**

"The source power calibration is complete."

**Severity:** Informational

**Further explanation:**

**Suggestions:**

**EventID:** 6802020C (hex)

**Message: 525**

"You have specified more than 7 standards for one or more calibration classes."

**Severity:** Informational

**Further explanation:** These have been truncated to 7 selections.

**EventID:** 6802020D (hex)

**Message: 526**

"No user calibration found for this channel."

**Severity:** Informational

**Further explanation:** A cal operation can not proceed until a calibration exists.

**Suggestions:** To find a calibration, you can select a Cal Set that contains the calibration needed for the current measurement.

**EventID:** 6802020E (hex)

**Message: 527**

"You do not need to acquire this standard for this calibration type."

**Severity:** Informational

**Further explanation:** This error can happen as a result of PROGRAMMATICALLY requesting the measurement of an un-needed calibration standard during a calibration procedure.

**Suggestions:** Check the specified cal type or eliminate the request for the measurement of the standard.

**EventID:** 6802020F (hex)

**Message: 528**

"Could not configure the Electronic Calibration system. Check to see if the module is plugged into the proper connector."

**Severity:** Informational

**Further explanation:** During an ECal operation, communication could not be established with the ECal module. The calibration will not be initiated until the presence of the ECal module is verified.

**Suggestions:** Verify the USB cable is connected properly. Disconnect and re-connect the cable to ensure the analyzer recognizes the module.

**EventID:** 68020210 (hex)

**Message: 529**

"DATA OUT OF RANGE: Design Limits Exceeded"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020211(hex)

**Message: 530**

"EXECUTION ERROR: Could not open ECal module memory backup file"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020212 (hex)

**Message: 531**

"EXECUTION ERROR: Access to ECal module memory backup file was denied"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020213 (hex)

**Message: 532**

"EXECUTION ERROR: Failure in writing to ECal module memory backup file"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020214 (hex)

**Message: 533**

"EXECUTION ERROR: Failure in reading from ECal module memory backup file"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020215 (hex)

**Message: 534**

"EXECUTION ERROR: Array index out of range"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020216 (hex)

**Message: 535**

"EXECUTION ERROR: Arrays wrong rank"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020217 (hex)

**Message: 536**

"EXECUTION ERROR: CPU"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020218 (hex)

**Message: 537**

"EXECUTION ERROR: Cannot ERASE module"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020219 (hex)

**Message: 538**

"EXECUTION ERROR: Cannot WRITE module"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E802021A (hex)

**Message: 539**

"EXECUTION ERROR: Entry Not Found"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E802021B (hex)

**Message: 540**

"EXECUTION ERROR: Invalid command while system is busy"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E802021C (hex)

**Message: 541**

"Electronic Cal: Unable to orient ECal module. Please ensure the module is connected to the necessary measurement ports."

**Severity:** Error

**Further explanation:** There is no RF connection to the ECal module during a calibration step. An ECal orientation measurement has been attempted but the signal was not found.

**Suggestions:** Connect the ECal module RF connections to ports specified for the calibration step. The ECal module typically requires at least -18dBm for measurements. If your measurement requires the power level to be less than that, clear the **Do orientation** checkbox to bypass the automatic detection step.

**EventID:** E802021D (hex)

**Message: 542**

"EXECUTION ERROR: NO SPACE for NEW CAL, DELETE A CAL"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E802021E (hex)

**Message: 543**

"EXECUTION ERROR: No More Room"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E802021F (hex)

**Message: 544**

"EXECUTION ERROR: Other array error"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020220 (hex)

**Message: 545**

"EXECUTION ERROR: Ranks not equal"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020221 (hex)

**Message: 546**

"EXECUTION ERROR: Too few CONSTANT ranks"

**Severity:** Error

**EventID:** E8020222 (hex)

**Message: 547**

"EXECUTION ERROR: Too few VARYing ranks"

**Severity:** Error

**EventID:** E8020223 (hex)

**Message: 548**

"EXECUTION ERROR: Unknown error"

**Severity:** Error

**EventID:** E8020224 (hex)

**Message: 549**

"EXECUTION ERROR: ecaldrvr.dll bug or invalid module #"

**Severity:** Error

**EventID:** E8020225 (hex)

**Message: 550**

"EXECUTION ERROR: unexpected error code from ecal driver"

**Severity:** Error

**EventID:** E8020226 (hex)

**Message: 551**

"EXECUTION ERROR: unexpected internal driver error"

**Severity:** Error

**EventID:** E8020227 (hex)

**Message: 552**

"HARDWARE ERROR: Can't access ECal Interface Module"

**Severity:** Error

**EventID:** E8020228 (hex)

**Message: 553**

"HARDWARE ERROR: Can't release LPT port, reboot"

**Severity:** Error

**EventID:** E8020229 (hex)

**Message: 554**

"HARDWARE ERROR: VNA Error"

**Severity:** Error

**EventID:** E802022A (hex)

**Message: 555**

"HARDWARE ERROR: not enough data read from ECal module"

**Severity:** Error

**EventID:** E802022B (hex)

**Message: 556**

"OPERATION ABORTED BY HOST COMPUTER"

**Severity:** Error

**EventID:** E802022C (hex)

**Message: 557**

"OPERATION ABORTED BY USER"

**Severity:** Error

**EventID:** E802022D (hex)

**Message: 558**

"OUT OF MEMORY"

**Severity:** Error

**EventID:** E802022E (hex)

**Message: 559**

"QUERY INTERRUPTED:Message(s Abandoned"

**Severity:** Error

**EventID:** E802022F (hex)

**Message: 560**

"QUERY UNTERMINATED: INCOMPLETE PROGRAM Message"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020230 (hex)

**Message: 561**

"QUERY UNTERMINATED: NOTHING TO SAY"

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020231 (hex)

**Message: 562**

"QUEUE OVERFLOW"

**Severity:** Error

**EventID:** E8020232 (hex)

**Message: 563**

"SETTINGS CONFLICT: ADDITIONAL STANDARDS ARE NEEDED"

**Severity:** Error

**EventID:** E8020233 (hex)

**Message: 564**

"SETTINGS CONFLICT: Adapter Cal is NOT possible"

**Severity:** Error

**EventID:** E8020234 (hex)

**Message: 565**

"SETTINGS CONFLICT: COMMAND OUT OF SEQUENCE"

**Severity:** Error

**EventID:** E8020235 (hex)

**Message: 566**

"SETTINGS CONFLICT: Cal STOPPED - VNA SETUP CHANGED"

**Severity:** Error

**EventID:** E8020236 (hex)



**Message: 567**

"SETTINGS CONFLICT: Calibration is NOT in progress"

**Severity:** Error

**EventID:** E8020237 (hex)

**Message: 568**

"SETTINGS CONFLICT: Can't find specified GPIB board"

**Severity:** Error

**EventID:** E8020238 (hex)

**Message: 569**

"SETTINGS CONFLICT: Can't find/load gpib32.dll"

**Severity:** Error

**EventID:** E8020239 (hex)

**Message: 570**

"SETTINGS CONFLICT: Can't find/load sicl32.dll"

**Severity:** Error

**EventID:** E802023A (hex)

**Message: 571**

"SETTINGS CONFLICT: Can't initialize VNA (bad address?)"

**Severity:** Error

**EventID:** E802023B (hex)

**Message: 572**

"SETTINGS CONFLICT: Can't load LPT port driver or USB driver DLL"

**Severity:** Error

**EventID:** E802023C (hex)

**Message: 573**

"SETTINGS CONFLICT: Invalid Calibration Sweep Mode."

**Severity:** Error

**EventID:** E802023D (hex)

**Message: 574**

"SETTINGS CONFLICT: Invalid Calibration Type"

**Severity:** Error

**EventID:** E802023E (hex)

**Message: 575**

"SETTINGS CONFLICT: Invalid Calibration"

**Severity:** Error

**EventID:** E802023F (hex)

**Message: 576**

"SETTINGS CONFLICT: Invalid GPIB board number specified"

**Severity:** Error

**EventID:** E8020240 (hex)

**Message: 577**

"SETTINGS CONFLICT: Invalid GPIB board type specified"

**Severity:** Error

**EventID:** E8020241 (hex)

**Message: 578**

"SETTINGS CONFLICT: Invalid Module Status"

**Severity:** Error

**EventID:** E8020242 (hex)

**Message: 579**

"SETTINGS CONFLICT: Invalid States"

**Severity:** Error

**EventID:** E8020243 (hex)

**Message: 580**

"SETTINGS CONFLICT: LPT port must be between 1 and 4"

**Severity:** Error

**EventID:** E8020244 (hex)

**Message: 581**

"Could not configure the Electronic Calibration system. Check to see if the module is properly connected."

**Severity:** Error

**EventID:** E8020245 (hex)

**Message: 582**

"SETTINGS CONFLICT: Specified LPT port does not exist"

**Severity:** Error

**EventID:** E8020246 (hex)

**Message: 583**

"SETTINGS CONFLICT: Use frequency domain for cal"

**Severity:** Error

**EventID:** E8020247 (hex)

**Message: 584**

"SETTINGS CONFLICT: Use step sweep type for cal."

**Severity:** Error

**EventID:** E8020248 (hex)

**Message: 585**

"SETTINGS CONFLICT: VNA address must be between 0 and 30"

**Severity:** Error

**EventID:** E8020249 (hex)

**Message: 586**

"SETTINGS CONFLICT: Wrong LPT port driver or USB driver DLL"

**Severity:** Error

**EventID:** E802024A (hex)

**Message: 587**

"SYNTAX ERROR: ECAL:DELAY command must have 2 numbers"

**Severity:** Error

**EventID:** E802024B (hex)

**Message: 588**

"SYNTAX ERROR: INCORRECT SYNTAX"

**Severity:** Error

**EventID:** E802024C (hex)

**Message: 589**

"SYNTAX ERROR: UNKNOWN COMMAND"

**Severity:** Error

**EventID:** E802024D (hex)

**Message: 590**

"Wrong port of module in RF path"

**Severity:** Error

**EventID:** E802024E (hex)

**Message: 591**

"User characterization not found in module"

**Severity:** Error

**EventID:** E802024F (hex)

**Message: 592**

**Severity:** Informational

"No source power calibration found for the channel and source port of the current measurement."

**Further explanation:** You tried to turn on source power cal but there is no source power cal data.

**Suggestions:** Perform a source power calibration

**EventID:** 68020250 (hex)

**Message: 593****Severity:** Informational

"A source power calibration sweep was not performed, so there is no correction for the channel and source port of the current measurement."

**Further explanation:** You tried to turn on source power cal but there is incomplete source cal data.**Suggestions:** Perform a complete source power calibration**EventID:** 68020251 (hex)**Message: 594****Severity:** Informational

"A new trace could not be added to the active window for viewing the source power cal sweep, because it would have exceeded the limit on number of traces/window. Please remove a trace from the window before proceeding with source power cal."

**Further explanation:** The source power cal attempts to add a data trace to the active window. The active window already contains four traces.**Suggestions:** Make the active window contain less than four traces.**EventID:** 68020252 (hex)**Message: 595****Severity:** Informational

"A new measurement could not be added for performing the source power cal sweep, because the limit on number of measurements has been reached. Please remove a measurement before proceeding with source power cal."

**Further explanation:** The source power cal attempts to add a measurement. The PNA already has the maximum number of measurements.**Suggestions:** Delete a measurement.**EventID:** 68020253 (hex)**Message: 596****Severity:** Informational

"The calibration power value associated with the source power calibration of Port %1 on Channel %2 was changed with the calibration on. The calibration was not turned off, but the power value might no longer represent the calibration."

**Further explanation:** The source power cal accuracy is questionable.**Suggestions:** If high accuracy is required, perform another source power calibration.**EventID:** 68020254 (hex)**Message: 597****Severity:** Informational

- Message that is passed from the power meter driver for a source power calibration. -

**Further explanation:** This error is generated by the power meter driver and passed through the PNA.**EventID:** 68020255 (hex)**Message: 598**

"During the acquisition of the sliding load standard, the slide was not properly moved to perform a circle fit. The

standard's raw impedance was used to determine the directivity for one or more points."

**Severity:** Informational

**Further Explanation:** To accurately characterize the standard, the sliding load must be move sufficiently to ensure enough samples around the complex circle or Smith Chart. Under-sampling will cause an inaccurate result.

**Suggestions:** For best results when using a sliding load, be sure to use multiple slide positions that cover the full range of movement from front to back of the slot.

**EventID:** 68020256 (hex)

**Message: 599**

"This feature requires an unused channel, but could not find one. Please free up a channel and try again."

**Severity:** Informational

**Further Explanation:** You attempted to view an item within a calset. However, the calset viewer requires that the result be displayed in a channel that is not currently in use. All the channels are currently used. The view can not display the requested item.

**Suggestions:** You must delete at least one channel that is currently in use.

**EventID:** 68020257 (hex)

**Message: 600**

"Interpolation of the original calibration is not allowed since it was performed using Segment Sweep. Correction has been turned off."

**Severity:** Informational

**EventID:** 68020258 (hex)

**Message: 601**

"Cal preferences saved. Cal preference settings can be changed from the 'Cal Preferences' drop down Cal menu."

**Severity:** Informational

**Further explanation:** [See Cal Preferences](#)

**EventID:** 68020259 (hex)

**Message: 608**

"CalType not set."

**Severity:** Error

**Further explanation:** A cal operation can not proceed until a calibration exists or the proper cal type is selected.

**Suggestions:** This error can happen if the calibration can't be found. To find a calibration, you can select a Cal Set that contains the calibration needed for the current measurements. This error can also happen if a calibration type is not specified before attempting to programmatically execute cal acquisitions. Specify the cal type before beginning a calibration procedure.

**EventID:** E8020260 (hex)

**Message: 609**

"The Calibration feature requested is not implemented."

**Further explanation:** The specified cal type can be one of many choices. For example, response calibrations require single standards, 1-Port calibrations require 3 standards, and 2-Port calibrations require up to 12 standards.

**Suggestions:** Be sure to measure only the standards needed for the specified cal type.

**EventID:** E8020261 (hex)

**Message: 610**

"The Calibration Class Acquisition requested is not valid for the selected Calibration Type. Please select a different acquisition or a different Calibration Type."

**EventID:** E8020262 (hex)

**Message: 611**

"The Calibration Standard data required for the selected caltype was not found."

**Severity:** Error

**Further explanation:** An unsuccessful attempt was made to retrieve a specified standard from the raw measurement buffer. The buffer should contain the raw measurements of cal standards stored during a calibration procedure.

**Suggestions:** Be sure the requested standard is required for the current cal type. Not all standards are needed for all cal types.

**EventID:** E8020263 (hex)

**Message: 612**

" The Error Term data required for the selected caltype was not found."

**Severity:** Error

**Further explanation:** An unsuccessful attempt was made to retrieve a specified error term from the error correction buffer. The buffer should contain the error correction arrays for the current calibration.

**Suggestions:** Be sure the requested error term is required for the current cal type. Not all error terms are needed for all cal types.

**EventID:** E8020264 (hex)

**Message: 613**

The Calibration data set was not found.

**Severity:** Error

**Further explanation:** An unsuccessful attempt to access a cal set has been made. This may indicate a calset has been deleted or has been corrupted.

**Suggestions:** Try again or select another cal set. If the cal set appears in the cal set list, it may need to be deleted.

**EventID:** E8020265 (hex)

**Message: 614**

"The specified measurement does not have a calibration valid for Confidence Check. Please select a different measurement, or recall or perform a different Calibration Type."

**Severity:** Error

**Further explanation:** The measurement choice is prevented so that calibration will not be turned off. Not all cal types support all measurements. For example, an 1-Port cal on S11 can not be used to calibrate an S12 measurement. When a measurement is selected that does not have a calibration which can be applied, an informational message is displayed and calibration is turned off.

**Suggestions:** Use a full 2-Port calibration to be compatible with any S-Parameter.

**EventID:** E8020266 (hex)

**Message: 615**

" New calset created."

**Severity:** Informational message.

**Further explanation:** The newly created cal set will be automatically named and time stamped. If this is the beginning of a calibration procedure, the cal set will not be stored to memory until the calibration has completed successfully. The new cal set will be deleted if the calibration is canceled or does not otherwise complete successfully.

**Suggestions:** Informational

EventID: 68020267

**Message: 617**

The calset file: <x> appears to be corrupted and cannot be removed. Exit the application, remove the file, and restart.

**Severity:** Error

**Suggestions:** The cal set file is stored in the application home directory C:\Program Files\Agilent\Network Analyzer\PNACalSets.dat. Remove this file, then restart the application.

**EventID:** E8020269 (hex)

**Message: 634**

"The calset file: <x> load failed."

**Severity:** Error

**Further explanation:** The calset file contains a collection of calsets. The file resides on the hard drive.

**Suggestions:** Try restarting the application. If the failure persists, you may have to delete the cal set data file and restart the application. The cal set file is stored in the application home directory. C:\Program Files\Agilent\Network Analyzer\PNACalSets.dat. Remove this file, then restart the application.

**EventID:** E802027A (hex)

**Message: 635**

"The calset file: <x> save failed."

**Severity:** Error

**Further explanation:** The file operation detected an error. The save operation was aborted.

**Suggestions:** Retry.

**EventID:** E802027B (hex)

**Message: 636**

"A calset was deleted."

**Severity:** Informational

**Further explanation:** One of the calsets has been successfully deleted from the collection of calsets available. This can happen as the result of a user request or intentional operation.

**Suggestions:** None

**EventID:** 6802027C (hex)

**Message: 637**

"The version of the calset file: <x> is not compatible with the current instrument."

**Severity:** Error

**Further explanation:** A versioning error can prevent a calset from being used. This can happen as a result of instrument firmware upgrades.

**Suggestions:** If the versioning error is the result of firmware upgrade, you will have to re-install the old version of firmware to re-use the calset file. Or you can re-create the calsets with the current version of firmware.

The cal set file is stored in the application home directory C:\Program Files\Agilent\Network Analyzer\PNACalSets.dat. Remove this file, then restart the application.

**EventID:** E802027D (hex)

**Message: 638**

"Incompatible CalSets found: <x> of <y> stored calsets have been loaded."

**Severity:** Error

**Further explanation:** Errors were found on some of the calsets stored in the calset file. The errors may have been caused by versioning issues that may have corrupted the various calset keys.

**Suggestions:** Use the calset viewer to look at the contents of calset files. Delete the files that are corrupted.

**EventID:** 6802027E (hex)

**Message: 639**

"The Calset file: <x> was not found. A new file has been created."

**Severity:** Informational

**Further explanation:** The calset file should be stored on the hard drive. When the application is started, a search is done and the file is loaded if it can be found. If the file is not found, the analyzer will create a new file and display this message.

**Suggestions:** None

**EventID:** 6802027F (hex)

**Message: 640**

"The Calset specified is currently in use."

**Severity:** Error

**Further explanation:** This may indicate a conflict between multiple calset users attempting calibration tasks.

**Suggestions:** Save the instrument state. Preset the analyzer and recall the instrument state. This may abort any processes that may be in progress.

**EventID:** E8020280 (hex)

**Message: 641**

"The calset specified has not been opened."

**Severity:** Error

**Further explanation:** Multiple users may be attempting to access the calset.

**Suggestions:** Close multiple calset users so that only one user will access the calset.

**EventID:** E8020281 (hex)

**Message: 642**

"The maximum number of cal sets has been reached. Delete old or unused cal sets before attempting to create new ones."

**Severity:** Error



**Suggestions:** You may also delete the calsets data file.

The cal set file is stored in the application home directory. C:\Program Files\Agilent\Network\_Analyzer\PNACalSets.dat. Remove this file, then restart the application.

**EventID:** E8020282 (hex)

**Message: 643**

The requested power loss table segment was not found.

**Severity:** Error

**EventID:** E8020283 (hex)

**Message: 644**

"A valid calibration is required before correction can be turned on."

**Severity:** Error

**Further explanation:** This usually indicates a calibration procedure has not run to completion or that the selected measurement does not have a valid calibration available from within the currently selected cal set.

**Suggestions:** To find a calibration, you can select a Cal Set that contains the calibration needed for the current measurements. This error can happen if a calibration type is not specified before attempting to programmatically execute cal acquisitions. Specify the cal type before beginning a calibration procedure.

**EventID:** E8020284 (hex)

**Message: 645**

The cal data for <x> is incompatible and was not restored. Please recalibrate."

**Severity:** Warning

**Further explanation:** None

**Suggestions:** None

**EventID:** A8020285 (hex)

**Message: 646**

"CalSet not loaded, version is too new."

**Severity:** Error

**Further explanation:** An old version of firmware is attempting to run with a new calset version. The version is incompatible.

**Suggestions:** The calset can be removed. You may also delete the calsets data file if you are migrating between various firmware revisions often and you would like to avoid this error. The cal set file is stored in the application home directory. C:\Program Files\Agilent\Network Analyzer\PNACalSets.dat. Remove this file, then restart the application.

**EventID:** E8020286 (hex)

**Message: 647**

"Custom cal type not found."

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E8020287 (hex)

**Message: 648**

"Custom correction algorithm defers to the client for interpolation."

**Severity:** Informational

**EventID:** 68020288 (hex)

**Message: 649**

"Custom cal dll threw an exception."

**Severity:** Error

**EventID:** E8020289 (hex)

**Message: 650**

"Could not load the ecal.dll library"

**Severity:** Error

**EventID:** E802028A (hex)

**Message: 656**

"The argument specified is not a valid cal type."

**Severity:** Error

**EventID:** E8020290 (hex)

**Message: 657**

"The function found existing interpolated data"

**Severity:** Informational

**EventID:** 68020291 (hex)

**Message: 658**

"The function computed new interpolation values."

**Severity:** Informational

**EventID:** 68020292 (hex)

**Message: 659**

"The source power measurement failed."

**Severity:** Error

**Suggestions:** Please check GPIB, power meter settings and sensor connections.

**EventID:** E8020293 (hex)

**Message: 660**

"Duplicate session found. Close session and retry."

**Severity:** Error

**EventID:** E8020294 (hex)

**Message: 661**

"The session does not exist. Open the session and try again."

**Severity:** Error

**Further explanation:**

**EventID:** E8020295 (hex)

**Message: 662**

"Attempt to launch a custom calibration failed."

**Severity:** Error

**Further explanation:**

**EventID:** E8020296 (hex)

**Message: 663**

"Request to measure a cal standard failed."

**Severity:** Error

**Further explanation:** Please ensure you are requesting to measure standards which are defined for this calibration.

**EventID:** E8020297 (hex)

**Message: 664**

"Since Electronic Calibration Kit is selected, Mechanical Cal Kit parameter cannot be changed."

**Severity:** Error

**Further explanation:**

**EventID:** E8020298 (hex)

**Message: 665**

"Frequencies of the active channel are below minimum or above maximum frequencies of the ECal module factory characterization."

**Suggestions:** Change the channel frequencies, or select another ECal module.

**Severity:** Error

**EventID:** E8020299 (hex)

**Message: 666**

"Calset chosen for characterizing the ECal Module Ports %1 does not contain a calibration for PNA Ports %2."

**Severity:** Error

**Suggestions:** Go back to select another calset or to perform another cal.

**EventID:** E802029A (hex)

**Message: 667**

"ECal module only has sufficient memory remaining to store a maximum of %1 points in User Characterization %2."

**Severity:** Error

**Suggestions:** Decrease your number of points, or choose to overwrite another user characterization.

**EventID:** E802029B (hex)

**Message: 668**

Input values are non-monotonic. Cannot interpolate.

**Severity:** Error

**EventID:** E802029C (hex)

**Message: 669**

Interpolation target is out of range. Cannot interpolate.

**Severity:** Error

**EventID:** E802029D (hex)

**Message: 670**

Guided Calibration Error: <>

**Severity:** Error

**EventID:** E802029E (hex)

**Message: 671**

The first call to the guided calibration interface must be Initialize.

**Severity:** Error

**EventID:** E802029F (hex)

**Message: 672**

The selected thru cal method was not recognized.

**Severity:** Error

**EventID:** E80202A0 (hex)

**Message: 673**

Could not generate the error terms.

**Severity:** Error

**EventID:** E80202A1 (hex)

**Message: 674**

Guided calibration must be performed on the active channel

**Severity:** Error

**EventID:** E80202A2 (hex)

**Message: 675**

You can not start using calibration steps until you have successfully called generate steps.

**Severity:** Error

**EventID:** E80202A3 (hex)

**Message: 676**

The step number given is out of range. Step numbers should be between 1 and the number of steps. 0 is not a valid step number.

**Severity:** Error

**EventID:** E80202A4 (hex)

**Message: 677**

A calset was selected for channel: <n> without restoring stimulus.

**Severity:** Informational

**EventID:** 680202A5 (hex)

**Message: 678**

A calset was selected for channel: <n> restoring stimulus.

**Severity:** Informational

**EventID:** 680202A6 (hex)

**Message: 679**

The selected calset stimulus could not be applied to the channel.

**Severity:** Informational

**EventID:** 680202A7 (hex)

**Message: 680**

You attempted to measure power at a frequency outside the frequency range defined for the specified power sensor. Select another sensor or adjust the range for this sensor.

**Severity:** Error

**EventID:** E80202A8 (hex)

**Message: 681**

Specified frequency is outside the frequency ranges currently defined for the power meter's sensors.

**Severity:** Error

**EventID:** E80202A9 (hex)

**Message: 682**

Additional Calibration Standards need to be acquired in order to calibrate over the entire frequency range currently being measured.

**Severity:** Informational

**EventID:** 680202AA (hex)

**Message: 683**

The PNA failed to convert cal kits for use by unguided calibrations. The recommended action is to restore Cal Kit defaults.

**Severity:** Error

**EventID:** E80202AB (hex)

**Message: 684**

The PNA failed to convert cal kits for use by unguided calibrations. CalKit defaults have been restored.

**Severity:** Error

**EventID:** E80202AC (hex)

**Message: 685**

Power meter is reserved by a source power cal acquisition already in progress.

**Severity:** Error

**EventID:** E80202AD (hex)

**Message: 686**

Source power calibration has not been performed or uploaded for the specified channel and source port.

**Severity:** Error

**EventID:** E80202AE (hex)

**Message: 687**

Source power calibration data array size for the specified channel and source port does not match it's associated stimulus number of points.

**Severity:** Error

**EventID:** E80202AF (hex)

**Message: 688**

Source power calibration of Port <n> on Channel <n> was turned off because the correction array no longer exists.

**Severity:** Error

**EventID:** E80202B0 (hex)

**Message: 689**

This command can only be used on a measurement created with a specified calibration loadport.

**Severity:** Error

**EventID:** E80202B1 (hex)

**Message: 690**

Interpolation is turned off and you have changed the stimulus settings of the original calibration, so correction has been turned off.

**Severity:** Error

**EventID:** E80202B2 (hex)

**Message: 691**

Stimulus settings for your current instrument state exceeded the parameters of the original calibration, so correction has been turned off.

**Severity:** Error

**EventID:** E80202B3 (hex)

**Message: 692**

Fixturing: the requested S2P file cannot be read. Possible formatting problem.

**Severity:** Error

**EventID:** E80202B4 (hex)

**Message: 693**

Fixturing: the requested S2P file cannot be opened.

**Severity:** Error

**EventID:** E80202B5 (hex)

**Message: 694**

Fixturing: the requested S2P file cannot be interpolated. This is usually because the frequency range in the file is a subset of the current channel frequency range.

**Severity:** Error

**EventID:** E80202B6 (hex)

**Message: 695**

Cal Registers can only be used by one channel: the channel conveyed in the name of the cal register. The name cannot be changed.

**Severity:** Error

Further explanation: See [Cal Registers](#)

**EventID:** E80202B7 (hex)

**Message: 696**

Fixturing: cannot be enabled with Response Calibrations and has been turned off.

**Severity:** Error

**EventID:** E80202B8 (hex)

**Message: 697**

The selected calibration cannot be performed for this measurement.

**Severity:** Error

**EventID:** E80202B9 (hex)

**Message: 698**

Fitting: RemoveAllConnectors() should be called prior to calling AddConnector after a fit has been attempted.

**Severity:** Error

**EventID:** E80202BA (hex)

**Message: 699**

An attempt was made to acquire calibration data before the system was properly initialized.

**Severity:** Error

**EventID:** E80202BB (hex)

**Message: 700**

Use IGuidedCalibration for multipoint calibration types.

**Severity:** Error

**EventID:** E80202BC (hex)

**Message: 701**

Guided calibration requires number of thru measurement paths be at least equal to the number of calibration ports minus 1.

**Severity:** Error

**EventID:** E80202BD (hex)

**Message: 702**

A thru path was specified that includes a port which the calibration was not specified to include.

**Severity:** Error

**EventID:** E80202BE (hex)

**Message: 703**

One or more of the ports to be calibrated was not found in the set of specified thru paths.

**Severity:** Error

**EventID:** E80202BF (hex)

---

**Hardware Errors**

---

**Message: 770**

Input power too high. Source power is off.

**Severity:** Warning

**EventID:** A8030302 (hex)

**Message: 771**

Source power restored.

**Severity:** Informational

**EventID:** 68030303 (hex)

**Message: 772**

"The spamnp.sys driver is not working. Check system hardware. ! Data will be simulated. !"

**Severity:** Error

**Further explanation:** The Network Analyzer application cannot locate the DSP board. Hardware or a driver may be malfunctioning. This is also common when attempting to run the Network Analyzer on a workstation.

**EventID:** E8030304 (hex)

**Message: 773**

"Instrument Serial Bus Not Working."

**Severity:** Error

**Further explanation:** The instrument EEPROM appears to contain either all ones or all zeros. A serial bus hardware failure prevents reading the EEPROM.

**EventID:** E8030305 (hex)

**Message: 848**

"Phase lock lost"

**Severity:** Error

**Further explanation:** The instrument source was not able to lock properly. This can be the result of broken hardware, poor calibration, or bad EEPROM values.

**Suggestions:** Perform source calibration. Click System / Service / Adjustments / Source Calibration



**EventID:** E8030350 (hex)

**Message: 849**

Phaselock restored.

**Severity:** Success

**EventID:** 0x28030351 (hex)

**Message: 850**

"Unknown hardware error."

**Severity:** Error

**Further explanation:** Hardware malfunctioned prevents communication with the DSP.

**EventID:** E8030352 (hex)

**Message: 851**

DSP communication lost.

**Severity:** Error

**EventID:** E8030353 (hex)

**Message: 852**

RF power off.

**Severity:** Error

**EventID:** E8030354 (hex)

**Message: 853**

RF power on.

**Severity:** Success

**EventID:** 28030355 (hex)

**Message: 854**

Hardware OK.

**Severity:** Success

**EventID:** 28030356 (hex)

**Message: 855**

"Source unlevelled."

**Severity:** Error

**Further explanation:** The source was unable to properly level at the requested power. The indicated power may not be accurate.

**Suggestions:** Try a different power level. Recalibrate source, if problem persists.

**EventID:** E8030357 (hex)

**Message: 856**

Source leveled.

**Severity:** Success

**EventID:** 28030358 (hex)

**Message: 857**

Input overloaded.

**Severity:** Error

**EventID:** E8030359 (hex)

**Message: 858**

Input no longer overloaded.

**Severity:** Success

**EventID:** 2803035A (hex)

**Message: 859**

"Yig calibration failed."

**Severity:** Error

**Further explanation:** Internal self-calibration of YIG oscillator tuning failed.

**EventID:** E803035B (hex)

**Message: 860**

Yig calibrated.

**Severity:** Success

**EventID:** 2803035C (hex)

**Message: 861**

"Analog ramp calibration failed."

**Severity:** Error

**Further explanation:** Internal analog sweep ramp calibration has failed.

**EventID:** E803035D (hex)

**Message: 862**

Analog ramp calibrated.

**Severity:** Success

**EventID:** 2803035E (hex)

**Message: 863**

Source temperature high.

**Severity:** Error

**EventID:** E803035F (hex)

**Message: 864**

Source temperature OK.

**Severity:** Success

**EventID:** 28030360 (hex)

**Message: 865**

"EEPROM write failed."

**Severity:** Error

**Further explanation:** Attempt to store calibration data to EEPROM has failed. There is a possible hardware failure.

**EventID:** E8030361 (hex)

**Message: 866**

EEPROM write succeeded.

**Severity:** Success

**EventID:** 28030362 (hex)

**Message: 867**

Attempted I/O write while port set to read only.

**Severity:** Error

**Further explanation:** Attempt to write to an I/O data port while the port set to input/read only.

**Suggestions:** Set data port to write/output before attempting to write to port.

**EventID:** E8030363 (hex)

**Message: 868**

" Attempted I/O read from write only port.

**Severity:** Error

**Further explanation:** Attempt to read from an I/O data port while the port set to output/write only.

**Suggestions:** Set data port to read/input before attempting to read from port.

**EventID:** E8030364 (hex)

**Message: 869**

Invalid hardware element identifier.

**Severity:** Error

**EventID:** E8030365 (hex)

**Message: 870**

Invalid gain level setting.

**Severity:** Error

**EventID:** E8030366 (hex)

**Message: 871**

Device driver was unable to allocate enough memory. Please try rebooting.

**Severity:** Error

**EventID:** E8030367 (hex)

**Message: 872**

DSP Error. Please Contact Agilent Support. Technical Information: DSP Type 1

**Severity:** Error

**EventID:** E8030368 (hex)

**Message: 873**

DSP Error. Please Contact Agilent Support. Technical Information: DSP Type 2

**Severity:** Error

**EventID:** E8030369 (hex)

**Message: 874**

DSP Error. Please Contact Agilent Support. Technical Information: DSP Type 3

**Severity:** Error

**EventID:** E803036A (hex)

**Message: 875**

DSP Error. Please Contact Agilent Support. Technical Information: DSP Type 4

**Severity:** Error

**EventID:** E803036B (hex)

**Message: 876**

DSP Error. Please Contact Agilent Support. Technical Information: DSP Type 5

**Severity:** Error

**EventID:** E803036C (hex)

**Message: 910**

The trigger connection argument was not recognized as valid by the firmware.

**Severity:** Error

**EventID:** 0xE803038E (hex)

**Message: 911**

The trigger connection specified does not support this trigger behavior

**Severity:** Error

**EventID:** E803038F (hex)

**Message: 912**

The trigger behavior specified was not recognized as valid by the firmware.

**Severity:** Error

**EventID:** E8030390 (hex)

**Message: 913**

The trigger connection specified does not physically exist on this network analyzer

**Severity:** Error

**EventID:** E8030391 (hex)

**Message: 914**

Cannot set "Accept Trigger Before Armed", since this hardware configuration does not support edge triggering.

**Severity:** Error

**EventID:** E8030392 (hex)

**Message: 915**

Cannot set "Trigger Output Enabled", since this hardware configuration does not support BNC2.

**Severity:** Error

**EventID:** E8030393 (hex)

**Message: 916**

Exceeded maximum trigger delay.

**Severity:** Error

**EventID:** E8030394 (hex)

**Message: 917**

Exceeded minimum trigger delay.

**Severity:** Error

**EventID:** E8030395 (hex)

---

## Measure Errors

---

**Message: 1024**

If you are going to display or otherwise use a memory trace, you must first store a data trace to memory.

**Severity:** Warning

**EventID:** A8040400 (hex)

**Message: 1025**

"The measurement failed to shut down properly. The application is in a corrupt state and should be shut down and restarted."

**Severity:** Error

**Further explanation:** This message is displayed if the PNA application becomes corrupt. If you continue to get this error, please call customer service

**EventID:** E8040401 (hex)

**Message: 1026**

The measurement failed to shut down properly. The update thread failed to exit properly.

**Severity:** Warning

**EventID:** A8040402 (hex)

**Message: 1027**

"Group Delay format with CW Time or Power sweeps produces invalid data."

**Severity:** Warning

**Further explanation:** Group Delay format is incompatible with single-frequency sweeps. Invalid data is produced.

**Suggestions:** Ignore the data or choose a different format or sweep type.

**EventID:** A8040403 (hex)

**Message: 1028**

**Severity:** Informational

"MSG\_LIMIT\_FAILED"

**Further explanation:** Limit line test failed.

**EventID:** 68040404 (hex)

**Message: 1029**

**Severity:** Informational

"MSG\_LIMIT\_PASSED"

**Further explanation:** Limit line test passed.

**EventID:** 68040405 (hex)

**Message: 1030**

"Exceeded the maximum number of measurements allowed."

**Severity:** Warning

**Further explanation:** See [Traces, Channels, and Windows on the PNA](#) for learn about maximum measurements.

**EventID:** A8040406 (hex)

**Message: 1031**

"Network Analyzer Internal Error. Unexpected error in AddNewMeasurement."

**Severity:** Warning

**Further explanation:** If you continue to get this message, contact product support.

**EventID:** A8040407 (hex)

**Message: 1032**

"No measurement was found to perform the selected operation. Operation not completed."

**Severity:** Warning

**Further explanation:** None

**Suggestions:**Create a measurement before performing this operation.

**EventID:** A8040408 (hex)

**Message: 1033**

The Markers All Off command failed.

**Severity:** Warning

**EventID:** A8040409 (hex)

**Message: 1034**

"A memory trace has not been saved for the selected trace. Save a memory trace before attempting trace math operations."

**Severity:** Warning

**Further explanation:** Must have a memory trace when trying to do Trace Math,

**EventID:** A804040A (hex)

**Message: 1035**

"MSG\_SET\_AVERAGE\_COMPLETE"

**Severity:** Informational

**Further explanation:** Informational for COM programming. Averaging factor has been reached.

**EventID:** 6804040B (hex)

**Message: 1036**

"MSG\_CLEAR\_AVERAGE\_COMPLETE"

**Further explanation:** Informational for COM programming. Averaging factor has NOT been reached.

**EventID:** 6804040C (hex)

**Message: 1037**

"Time Domain transform requires at least 3 input points. The transform has been deactivated."

**Severity:** Informational

**Further explanation:** None

**Suggestions:** Increase the number of points.

**EventID:** 6804040D (hex)

**Message: 1038**

Smoothing requires a scalar format, and has been deactivated.

**Severity:** Informational

**EventID:** 6804040E (hex)

**Message: 1039**

A receiver power calibration in this instrument state file cannot be recalled into this firmware version.

**Severity:** Warning

**EventID:** A804040F (hex)

**Message: 1104**

"Exceeded limit on number of measurements."

**Severity:** Error

**Further explanation:** See [Traces, Channels, and Windows on the PNA](#) for measurement limits.

**EventID:** E8040450 (hex)

**Message: 1105**

"Parameter not valid."

**Severity:** Error

**Further explanation:** A measurement parameter that was entered programmatically is not valid.

**EventID:** E8040451 (hex)

**Message: 1106**

"Measurement not found."

**Severity:** Error

**Further explanation:** Any of these could be the cause:

Trying to calibrate but already have maximum measurements.

Trying to do a confidence check but there is not a measurement.

Trying to create, activate, or alter a measurement through COM that has been deleted through the front panel.

Trying to use a trace name through programming that is not unique.

**EventID:** E8040452 (hex)

**Message: 1107**

"No valid memory trace."

**Severity:** Error

**Further explanation:** Must have a memory trace when trying to do Trace Math,

**Suggestions:** Store a memory trace.

**EventID:** E8040453 (hex)

**Message: 1108**

"The reference marker was not found."

**Severity:** Error

**Further explanation:** Attempted to create a delta marker without first creating a reference marker (COM only).

**EventID:** E8040454 (hex)

**Message: 1109**

"Data and Memory traces are no longer compatible. Trace Math has been turned off."

**Severity:** Error

**Further explanation:** Warning - channel setting has changed while doing trace math.

**Suggestions:** Store another memory trace and turn trace math back on.

**EventID:** A8040455 (hex)

**Message: 1110**

"Data and Memory traces are not compatible. For valid trace math operations, memory and data traces must have similar measurement conditions."

**Severity:** Error

**Further explanation:** Tried to do trace math without compatible data and memory traces.

**Suggestions:** Store another memory trace.

**EventID:** E8040456 (hex)

**Message: 1111**

"Marker Bandwidth not found."

**Severity:** Error

**Further explanation:** Could not find a portion of trace that meets the specified bandwidth criteria.

**EventID:** E8040457 (hex)



**Message: 1112**

"The peak was not found."

**Severity:** Error

**Further explanation:** Could not find portion of trace that meets peak criteria.

**Suggestions:** See Marker Peak criteria.

**EventID:** E8040458 (hex)

**Message: 1113**

"The target search value was not found."

**Severity:** Error

**Further explanation:** Could not find interpolated data point that meets search value.

**EventID:** E8040459 (hex)

**Message: 1114**

"Reflection measurement, such as S11, must supply an auxiliary port to disambiguate 2-port measurements on multiport instruments."

**Severity:** Error

**Further explanation:**

**EventID:** E804045A (hex)

**Message: 1115**

"The receiver power calibration has been turned off because the type of measurement or source port has changed, so the calibration is no longer valid."

**Severity:** Warning

**Further explanation:**

**EventID:** A804045B (hex)

**Message: 1116**

"Receiver power cal requires the active measurement to be of unratiod power."

**Severity:** Warning

**Further explanation:**

**EventID:** A804045C (hex)

**Message: 1117**

"There is currently no source power calibration associated with the channel and source port of the active measurement. A source power cal should be performed or recalled before performing a receiver power calibration."

**Severity:** Warning

**Further explanation:**

**EventID:** A804045D (hex)

**Message: 1118**

"The attempted operation can only be performed on a standard measurement type."

**Severity:** Error

**Further explanation:**

**EventID:** E804045E (hex)

**Message: 1119**

"The custom measurement cannot be loaded because it is not compatible with the Network Analyzer hardware."

**Severity:** Error

**Further explanation:**

**Suggestions:**

**EventID:** E804045F (hex)

**Message: 1120**

"The custom measurement cannot be loaded because it is not compatible with the Network Analyzer software."

**Severity:** Error

**Further explanation:**

**EventID:** E8040460 (hex)

**Message: 1121**

"The custom measurement load operation failed for an unspecified reason."

**Severity:** Error

**Further explanation:**

**EventID:** E8040461 (hex)

**Message: 1122**

"The custom measurement data processing has generated an unhandled exception, and will be terminated. The PNA software may be in an unstable state and it is recommended that the PNA software be shutdown and restarted."

**Severity:** Error

**Further explanation:**

**EventID:** E8040462 (hex)

**Message: 1123**

"The attempted operation can only be performed on a custom measurement type."

**Severity:** Error

**Further explanation:**

**EventID:** E8040463 (hex)

**Message: 1124**

"The requested custom measurement is not available."

**Severity:** Error

**Further explanation:**

**EventID:** E8040464 (hex)

**Message: 1125**

"The requested custom algorithm was not found."

**Severity:** Error

**Further explanation:**

**EventID:** E8040465 (hex)

**Message: 1126**

"Normalization cannot be turned on because the measurement does not have a valid divisor buffer."

**Severity:** Error

**Further explanation:**

**EventID:** E8040466 (hex)

**Message: 1127**

"The Raw Data requested by the measurement could not be provided."

**Severity:** Warning

**Further explanation:**

**EventID:** A8040467 (hex)

**Message: 1128**

"The selected Sweep Type does not allow Transform and Gating. Transform and Gating disabled. "

**Severity:** Error

**Further explanation:**

**EventID:** E8040468 (hex)

**Message: 1129**

Memory trace can not be applied to this measurement

**Severity:** Error

**EventID:** E8040469 (hex)

**Message: 1130**

Normalization can not be applied to this measurement

**Severity:** Error

**EventID:** E804046A (hex)

**Message: 1131**

The data provided has an invalid number of points. It could not be stored

**Severity:** Error

**EventID:** E804046B (hex)

**Message: 1132**

The measurement stored in the save/recall state has an invalid version. It could not be loaded

**Severity:** Error

**EventID:** E804046C (hex)

**Message: 1133**

This data format argument for this operation must be "naDataFormat\_Polar"

**Severity:** Error

**EventID:** E804046D (hex)

**Message: 1134**

This data format argument for this operation must be a scalar data format

**Severity:** Error

**EventID:** E804046E (hex)

**Message: 1135**

The memory trace is not valid for the current measurement setup.

**Severity:** Error

**EventID:** E804046F (hex)

**Message: 1136**

This measurement is incompatible with existing measurements in this channel. Choose another channel.

**Severity:** Error

**EventID:** E8040470 (hex)

**Message: 1137**

Port extension correction is not available for offset frequency measurements. Port extension correction has been disabled.

**Severity:** Error

**EventID:** E8040471 (hex)

**Message: 1138**

Physical port number assignments for logical port mappings must be unique.

**Severity:** Error

**EventID:** E8040472 (hex)

---

**Parser Errors**

---

**Message: 1281**

"You have sent a read command to the analyzer without first requesting data with an appropriate output command. The analyzer has no data in the output queue to satisfy the request."

**Severity:** Error

**EventID:** 68050501 (hex)

**Message: 1282**

"You must remove the active controller from the bus or the controller must relinquish the bus before the analyzer can assume the system controller mode."

**Severity:** Error

**EventID:** E8050502(hex)

**Message: 1283**

"The analyzer did not receive a complete data transmission. This is usually caused by an interruption of the bus transaction."

**Severity:** Error

**EventID:** E8050503 (hex)

**Message: 1284**

"The instrument status byte has changed."

**Severity:** Informational

**EventID:** 68050504 (hex)

**Message: 1285**

"The SCPI command received has caused error number %1: "%2"."

**Severity:** Informational

**EventID:** 68050505 (hex)

**Message: 1286**

"The INET LAN server has been started as process number %1."

**Severity:** Informational

**EventID:** 68050506 (hex)

**Message: 1360**

"Execution of the SCPI command has failed"

**Severity:** Error

**EventID:** E8050550 (hex)

**Message: 1361**

" The INET/LAN device is not accessible."

**Severity:** Error

**EventID:** E8050551 (hex)

**Message: 1362**

"The INET/LAN driver was not found. "

**Severity:** Error

**EventID:** E8050552 (hex)

**Message: 1363**

"The INET/LAN driver was not found."

**Severity:** Error

**EventID:** E8050553 (hex)

**Message: 1364**

"The INET/LAN device is unable to acquire the necessary resources. "

**Severity:** Error

**EventID:** E8050554 (hex)

**Message: 1365**

"The INET/LAN device generated a generic system error. "

**Severity:** Error

**EventID:** E8050555 (hex)

**Message: 1366**

"Invalid address for the INET/LAN device."

**Severity:** Error

**EventID:** E8050556 (hex)

**Message: 1367**

"The INET I/O library was not found. "

**Severity:** Error

**EventID:** E8050557 (hex)

**Message: 1368**

"An error occurred in the INET system. "

**Severity:** Error

**EventID:** E8050558 (hex)

**Message: 1369**

"Access to the INET/LAN driver was denied. "

**Severity:** Error

**EventID:** E8050559 (hex)

**Message: 1370**

"Could not load error system message dll."

**Severity:** Error

**EventID:** E805055A (hex)

**Message: 1371**

"ErrorMessage.dll does not export the right function."

**Severity:** Error

**EventID:** E805055B (hex)

**Message: 1372**

"Custom scpi library was not able to be knitted"

**Severity:** Error

**EventID:** E805055C (hex)

**Message: 1373**

"Could not knit the scpi error messages from the ErrorMessage lib"

**Severity:** Error

**EventID:** E805055D (hex)

**Message: 1374**

Command is obsolete with this software version.

**Severity:** Error

**EventID:** E808055E (hex)

**Message: 1375**

CALC measurement selection set to none. Use [Calc:Par:Sel](#)

**Severity:** Error

**EventID:** E808055F (hex)

**Message: 1535**

"Parser got command: %1."

**Severity:** Informational

**EventID:** 680505FF (hex)

---

## Display Errors 1536 - 1621

---

**Message: 1536**

"Exceeded the maximum of 4 traces in each window. The trace for <x> will not be added to window <x>."

**Severity:** Warning

**Further explanation:** None

**Suggestions:** Create the trace in another window. See the [PNA window limits](#).

**EventID:** A8060600 (hex)

**Message: 1537**

"Exceeded the maximum of 16 data windows. New window will not be created."

**Severity:** Warning

**Further explanation:** None

**Suggestions:** Create the trace in an existing window. See the [PNA window limits](#).

**EventID:** A8060601 (hex)

**Message: 1538**

"No Data Windows are present. Unable to complete operation."

**Severity:** Warning

**Further explanation:** Your remote SCPI operation tried to create a new measurement while there were no windows present

**Suggestions:** Create a new window before creating the measurement. See example [Create a measurement using SCPI](#)

**EventID:** A8060602 (hex)

**Message: 1539**

"No data traces are present in the selected window. Operation not completed."

**Severity:** Warning

**Further explanation:** None

**EventID:** A8060603 (hex)

**Message: 1540**

"Cannot complete request to arrange existing measurements in <x> windows due to the limit of <x> traces per window."

**Severity:** Informational

**Further explanation:** The arrange window feature cannot put the existing traces into the number of windows you requested because only 4 traces per window are allowed. [See Arranging Existing Measurements](#)

**Suggestions:** Either create more windows or delete some traces.

**EventID:** 68060604 (hex)

**Message: 1541**

"Unable to establish a connection with the specified printer."

**Severity:** Warning

**Further explanation:** None

**Suggestions:** Refer to Printer Help

**EventID:** A8060605 (hex)

**Message: 1542**

"Printout canceled."

**Severity:** Informational

**EventID:** 68060606 (hex)

**Message: 1616**

"Window not found."

**Severity:** Error

**Further explanation:** A window was specified in your program which does not exist.

**Suggestions:** Query the name of your window before specifying.

**EventID:** E8060650 (hex)

**Message: 1617**

"Duplicate window ID specified."

**Severity:** Error

**Further explanation:** None

**EventID:** E8060651 (hex)

**Message: 1618**

"Exceeded limit on number of windows."

**Severity:** Error

**Further explanation:** There is a limit of 4 windows per screen.



**EventID:** E8060652 (hex)

**Message: 1619**

"Exceeded limit on number of traces/window."

**Severity:** Error

**Further explanation:** There is a limit of 4 traces per window. See the [Traces, Channels, and Windows on the PNA](#).

**Suggestions:** Create the trace in another window

**EventID:** E8060653 (hex)

**Message: 1620**

"Trace not found."

**Severity:** Error

**Further explanation:** Your program tried to communicate with a non-existing trace.

**Suggestions:** Query the trace ID before writing to it.

**EventID:** E8060654 (hex)

**Message: 1621**

"The operating system does not recognize this printer."

**Severity:** Warning

**EventID:** A8060655 (hex)

**Message: 1622**

Duplicate trace ID specified.

**Severity:** Error

**EventID:** E8060656 (hex)

---

**Channel Errors 1792 -1878**

---

**Message: 1792**

"Sweep Complete."

**Severity:** Informational

**Further explanation:** None

**Suggestions:**None

**EventID:** 68070700 (hex)

**Message: 1793**

"All triggerable acquisitions have completed."

**Severity:** Informational

**Further explanation:**

**EventID:** 68070701 (hex)

**Message: 1794**

"The last trigger produced an aborted sweep."

**Severity:** Informational

**Further explanation:**

**EventID:** 68070702 (hex)

**Message: 1795**

"The segment list must be adjusted to have at least one active segment with more than 0 points to use segment sweep."

**Severity:** Informational

**Further explanation:** You attempted to change **Sweep type** to Segment sweep, but there is either no segments defined or no sweep points in the defined segments

**Suggestions:** Define at least one segment with at least one measurement point. See Segment sweep for more information

**EventID:** 68070703 (hex)

**Message: 1796**

"MSG\_SET\_CHANNEL\_DIRTY"

**Severity:** Informational

**Further explanation:** This informational message occurs when a channel setting has changed but the channel still has data that was taken with the previous setting. The following CLEAR message occurs when new channel data is taken.

**EventID:** 68070704 (hex)

**Message: 1797**

"MSG\_CLEAR\_CHANNEL\_DIRTY"

**Severity:** Informational

**Further explanation:** The previous SET message occurs when a channel setting has changed but the channel still has data that was taken with the previous setting. This CLEAR message occurs when new channel data is taken.

**EventID:** 68070705 (hex)

**Message: 1798**

Sweep time has changed from Auto to Manual mode. If desired to return to Auto mode, enter sweep time value of 0.

**Severity:** Informational

**EventID:** 68070706 (hex)

**Message: 1799**

"Set Sweep Completed"

**Severity:** Informational

**Further explanation:** This event occurs when a sweep and it's associated sweep calculations finish. This is typically when all sweeps on a channel complete.

**EventID:** 68070707 (hex)

**Message: 1800**

"Clear Sweep Completed"

**Severity:** Informational

**Further explanation:** This event occurs immediately after the SET SWEEP COMPLETED event. These two events set and clear the "Sweep Completed" bit (bit 4) on the SCPI Device Status register.

**EventID:** 68070708 (hex)

**Message: 1801**

"All Sweeps Completed and Processed"

**Severity:** Informational

**Further explanation:** This event occurs when all of the sweeps and sweep calculations are complete for a channel.

**EventID:** 68070709 (hex)

**Message: 1802**

Low Pass : Frequency limits have been changed.

**Severity:** Informational

**EventID:** 6807070A (hex)

**Message: 1803**

Low Pass : Number of points have been changed.

**Severity:** Informational

**EventID:** 6807070B (hex)

**Message: 1804**

Low Pass : Frequency limits and number of points have been changed.

**Severity:** Informational

**EventID:** 6807070C (hex)

**Message: 1872**

"Channel not found."

**Severity:** Error

**Further explanation:** A non-existent channel is being referenced under program control.

**Suggestions:** Query the channel number, then refer to it by number.

**EventID:** E8070750 (hex)

**Message: 1873**

"The requested sweep segment was not found."

**Severity:** Error

**Further explanation:** A non-existent sweep segment is being referenced under program control.

**EventID:** E8070751 (hex)

**Message: 1874**

"The sweep segment list is empty."

**Severity:** Error

**Further explanation:** Segment Sweep cannot be specified unless there is at least one defined segment. This error will only occur under remote control.

**EventID:** E8070752 (hex)

**Message: 1875**

"The number of points in active sweep segment list segments is 0."

**Severity:** Error

**Further explanation:** Segment Sweep cannot be specified unless there is at least data point specified in a segment. This error will only occur under remote control.

**EventID:** E8070753 (hex)

**Message: 1876**

"The specified source attenuator is not valid."

**Severity:** Error

**Further explanation:** You tried to set the Attenuator property on the Channel object on a PNA that doesn't have a source attenuator.

**EventID:** E8070754 (hex)

**Message: 1877**

"Log Frequency sweep cannot be selected with the current Number of Points. Please reduce Number of Points."

**Severity:** Error

**Further explanation:** The maximum number of points that can be used for Log sweep is 401.

**EventID:** E8070755 (hex)

**Message: 1878**

"The requested Number of Points is greater than can be selected for Log Frequency sweep."

**Severity:** Error

**Further explanation:** The maximum number of points that can be used for Log sweep is 401.

**EventID:** E8070756 (hex)

**Message: 1879**

"Response frequencies exceeded instrument range so Frequency Offset has been turned off."

**Severity:** Error

**Further explanation:** This error is returned whenever the instrument detects that the stimulus sweep setup and Frequency Offset settings result in computed response frequencies that exceed instrument limits. When this occurs, the instrument automatically turns off Frequency Offset to avoid the out-of-range conditions.

**Suggestions:** When this condition has occurred, change settings for either the stimulus frequencies or Frequency Offset so that the Response frequencies are within instrument bounds. Once this is done, Frequency Offset can once again be turned on.

**EventID:** E8070757 (hex)

**Message: 1880**

The total number of points for all the given segments exceeds the maximum number of points supported. The segments were not changed.

**Severity:** Error

**EventID:** E8070758 (hex)

**Message: 1881**

This instance of the Channels object was not used to place the channels in Hold, so no channels were resumed.

**Severity:** Error

**EventID:** E8070759 (hex)

**Message: 1882**

The port number was outside the range of allowed port numbers.

**Severity:** Error

**EventID:** E807075A (hex)

**Message: 1883**

More ports than are present are required for this operation.

**Severity:** Error

**EventID:** E807075B (hex)

---

**General Errors**

---

**Message: 2048**

"The function you requested requires a capability provided by an option to the standard analyzer. That option is not currently installed."

**Severity:** Error

**Further explanation:** None

**Suggestions:**To view the options on your analyzer, click **Help \ About Network Analyzer**. For more information see [PNA Options](#)

**EventID:** 68080800 (hex)

**Message: 2049**

"The feature you requested is not available on the current instrument."

**Severity:** Error

**Further explanation:** None

**EventID:** 68080801 (hex)

**Message: 2050**

"The feature you requested is incompatible with the current instrument state."

**Severity:** Error

**Further explanation:** None

**Suggestions:** None

**EventID:** 68080802 (hex)

**Message: 2051**

"File<x> has been saved."

**Severity:** Informational

**Further explanation:** None

**EventID:** 68080803 (hex)

**Message: 2052**

"Attempt to save <x> failed."

**Severity:** Error

**Further explanation:** None

**Suggestions:** If using a floppy disk, ensure it is inside the drive and the disk is not full. Check the filename for special characters.

**EventID:** E8080804 (hex)

**Message: 2053**

"Attempt to recall file failed because <x> was not found."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080805 (hex)

**Message: 2054**

"<x> has a bad header."

**Severity:** Error

**Further explanation:** None

**Suggestions:** Recopy the file and / or delete the file.

**EventID:** E8080806 (hex)

**Message: 2056**

"Request to enter hibernate state."

**Further explanation:** None

**EventID:** 68080808 (hex)

**Message: 2057**

"Power up from automatic hibernate state. Program received PBT\_APMRESUMEAUTOMATIC Message."

**Further explanation:** None

**EventID:** 68080809 (hex)

**Message: 2058**

"Power up from suspend hibernate state. Program received PBT\_APMRESUMESUSPEND Message."

**Further explanation:** None

**EventID:** 6808080A (hex)

**Message: 2059**

"Power up from suspend hibernate state. Program received PBT\_APMRESUMECRITICAL Message."

**Severity:** Warning

**Further explanation:** None

**EventID:** A808080B (hex)

**Message: 2060**

"Power up from unknown hibernate state UI recovery called. Program received no PBT\_Message within the time allotted and is attempting recovery."

**Severity:** Warning

**Further explanation:** None

**EventID:** A808080C (hex)

**Message: 2061**

"<x> already exists. File is being overwritten."

**Further explanation:** Used only for remote applications

**EventID:** 6808080D (hex)

**Message: 2062**

"File has not been saved."

**Severity:** Error

**Further explanation:** Used only for remote applications

**EventID:** E808080E (hex)

**Message: 2063**

"File <x> has been recalled."

**Further explanation:** Used only for remote applications

**EventID:** 6808080F (hex)

**Message: 2064**

"State version in <x> is considered obsolete by this version of this code."

**Severity:** Error

**Further explanation:** You attempted to recall a file that is no longer valid.

**Suggestions:** You must recreate the file manually.

**EventID:** E8080810 (hex)

**Message: 2065**

"State version in <x> is newer than the latest version supported by this code."

**Severity:** Error

**Further explanation:** You attempted to recall a file that was created by a later version of the PNA application.

**Suggestions:** You must recreate the file manually.

**EventID:** E8080811 (hex)

**Message: 2066**

"Error occurred while reading file <x>"

**Severity:** Error

**Further explanation:** The file may be corrupt.

**Suggestions:** Try to recreate the file.

**EventID:** E8080812 (hex)

**Message: 2067**

"Windows shell error: <x>"

**Severity:** Error

**Further explanation:** None

**EventID:** E8080813 (hex)

**Message: 2068**

Send message timed out returning: <x>.

**Severity:** Error

**Further explanation:** None

**EventID:** E8080814 (hex)

**Message: 2069**

"Changing GPIB mode to System Controller."

**Severity:** Informational

**Further explanation:** None

**EventID:** 68080815 (hex)

**Message: 2070**

"Changing GPIB mode to Talker Listener."

**Severity:** Informational

**Further explanation:** None

**EventID:** 68080816 (hex)

**Message: 2071**

"The Network Analyzer can not be put in GPIB System Controller mode until the GPIB status is Local. Stop any remote GPIB programs which may be using the Network analyzer, press the Macro/Local key and try again. "

**Severity:** Informational

**Further explanation:** See [LCL and RMT Operation](#)

**Suggestions:** Press the Macro/Local key and try again.

**EventID:** 68080817 (hex)

**Message: 2120**

"This method can not be invoked through a late-bound COM call."

**Severity:** Error

**Further explanation:** None

**Suggestions:** Use the alternate method described in the [COM programming documentation](#)

**EventID:** E8080878 (hex)



**Message: 2128**

"The specified format is invalid."

**Severity:**Error

**Further explanation:** None

**EventID:** E8080850 (hex)

**Message: 2129**

"WINNT exception caught by Automation layer."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080851 (hex)

**Message: 2130**

"Bad port specification."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080852 (hex)

**Message: 2131**

"Failed to find a printer."

**Severity:** Error

**Further explanation:** None

**Suggestions:** See [Connecting to a Printer](#)

**EventID:** E8080853 (hex)

**Message: 2132**

"Manual trigger ignored."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080854 (hex)

**Message: 2133**

"Attempt to set trigger failed."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080855 (hex)

**Message: 2134**

"Macro execution failed."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080856 (hex)

**Message: 2135**

"Specified macro definition is incomplete."

**Severity:** Error

**Further explanation:**

**EventID:** E8080857 (hex)

**Message: 2137**

"Block data length error."

**Severity:** Error

**Further explanation:** See [Getting Data from the Analyzer](#)

**EventID:** E8080859 (hex)

**Message: 2139**

"Requested data not found."

**Severity:** Error

**Further explanation:** None

**EventID:** E808085B (hex)

**Message: 2142**

"The parameter supplied was out of range, so was limited to a value in range before being applied to the instrument."

**Severity:** Success

**Further explanation:** None

**Suggestions:** View range limits before sending programming commands.

**EventID:** 2808085E (hex)

**Message: 2143**

The parameter supplied was out of range, so was limited to a value in range before being applied to the instrument.

**Severity:** Error

**EventID:** E808085F (hex)

**Message: 2144**

"Request failed. The required license was not found."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080860 (hex)

**Message: 2145**

"A remote call to the front panel has returned hresult <x>"

**Severity:** Error

**Further explanation:** This may indicate a problem with the front panel

**Suggestions:** Contact Technical support

**EventID:** E8080861 (hex)

**Message: 2146**

The recall operation failed.

**Severity:** Error

**Further explanation:**

**EventID:** E8080862 (hex)

**Message: 2147**

Attempt to save file failed.

**Severity:** Error

**Further explanation:**

**EventID:** E8080863 (hex)

**Message: 2148**

Recall attempt failed because file was not found.

**Severity:** Error

**Further explanation:**

**EventID:** E8080864 (hex)

**Message: 2149**

Recall file has a bad header.

**Severity:** Error

**Further explanation:**

**EventID:** E8080865 (hex)

**Message: 2150**

Recall file version is obsolete and no longer compatible with this instrument.

**Severity:** Error

**Further explanation:**

**EventID:** E8080866 (hex)

**Message: 2151**

The recall file contains an istate version newer than this instrument. A remote call to the front panel has returned hresult %1

**Severity:** Error

**Further explanation:**

**EventID:** E8080867 (hex)

**Message 2152**

"Front Panel <x>

**Severity:** Error

**Further explanation:** None

**EventID:** E8080868 (hex)

**Message 2153**

"Front Panel message"

**Severity:** Informational

**Further explanation:** None

**EventID:** 68080869 (hex)

**Message 2154**

"Power Service <x>

**Severity:** Error

**Further explanation:** There is more than 1 instance of powerservice running. There should only be one running. This might happen after running install shield - especially when upgrading the CPU board.

**Suggestions:** Try rebooting. If this persists, please call Customer Support.

**EventID:** E808086A (hex)

**Message 2155**

"Power Service <x>

**Severity:** Informational

**Further explanation:** None

**EventID:** 6808086B (hex)

**Message 2156**

"The Agilent Technologies GPIB driver can not be loaded or unloaded."

**Severity:** Error

**Further explanation:** None

**Suggestions:** If the problem persists, from the PNA desktop, right-click on My Computer. Click Properties, Click Hardware Tab. Click Device Manager Button. Expand GPIB Devices. Right-click and click Uninstall all GPIB interfaces devices. Reboot the PNA.

**EventID:** E808086C (hex)

**Message 2157**

"The National Instruments GPIB driver can not be loaded or unloaded."

**Severity:** Error

**Further explanation:** None

**Suggestions:** If the problem persists, from the PNA desktop, right-click on My Computer. Click Properties, Click Hardware Tab. Click Device Manager Button. Expand GPIB Devices. Right-click and click Uninstall all GPIB interfaces devices. Reboot the PNA.

**EventID:** E808086D (hex)

**Message 2158**

"The Agilent GPIB driver is loaded but it can not start its parser."

**Severity:** Error

**Further explanation:** None

**EventID:** E808086E (hex)

**Message: 2159**

The front panel is in remote mode.

**Severity:** Warning

**EventID:** A808086F (hex)

**Message: 2160**

The Registry Key specified could not be found.

**Severity:** Error

**EventID:** E8080870 (hex)

**Message: 2161**

An overcurrent condition has been detected on a probe plugged into the front panel.

**Severity:** Warning

**EventID:** A8080871 (hex)

**Message: 2162**

The operation timed out.

**Severity:** Error

**EventID:** E8080872 (hex)

**Message 2163**

"The Network Analyzer executed a preset."

**Severity:** Informational

**Further explanation:** None

**EventID:** 68080873 (hex)

**Message 2164**

"Access to file denied."

**Severity:** Error

**Further explanation:** This means that the system can not open an output file for writing. Most likely because the file is write protected.

**Suggestions:** Pick another file name or file directory, check floppy disk hard disk write access.

**EventID:** E8080874 (hex)

**Message 2165**

"File type is structured storage."

**Severity:** Informational

**Further explanation:** None

**EventID:** 68080875 (hex)

**Message 2166**

"The trigger operation failed."

**Severity:** Error

**Further explanation:** None

**EventID:** E8080876 (hex)

**Message 2167**

"Argument out of range error."

**Severity:** Error

**Further explanation:** None

**Suggestions:** None

**EventID:** E8080877 (hex)

**Message: 2169**

The given COM object is not a custom application

**Severity:** Error

**EventID:** E8080879 (hex)

**Message: 2170**

The eventID supplied was not recognized as a valid PNA eventID

**Severity:** Error

**EventID:** E808087A (hex)

**Message: 2171**

The operation was canceled.

**Severity:** Error

**EventID:** E808087B (hex)

**Message: 2172**

High security level cannot be disabled directly. Only an instrument preset or recall of lower security instrument state will reset this security level.

**Severity:** Error

**EventID:** E808087C (hex)

**Message: 2173**

Local lockout mode is on. The PNA application will not accept input from front panel, keyboard or mouse until this mode is turned off from a remote interface.

**Severity:** Error

**EventID:** E808087D (hex)

**Message: 2174**

The SnP request is not valid for the selected measurement.

**Severity:** Error

**EventID:** E808087E (hex)

**Message: 2175**

Preset is not supported while this dialog or wizard is open. Close the dialog or wizard and then try again.

**Severity:** Error

**EventID:** E808087F (hex)

**Message: 2176**

The function you requested requires a capability provided by an option to the standard analyzer. That option is not currently installed.

**Severity:** Error

**EventID:** E8080880 (hex)

**Message: 2177**

Catastrophic error. Crash dump recorded at <n>

**Severity:** Error

**EventID:** E8080881 (hex)

**Message: 2178**

<n>

**Severity:** Error

**EventID:** E8080882 (hex)

**Message: 2179**

Failed to open gen.lic.

**Severity:** Error

**EventID:** E8080883 (hex)

## About Error Messages

---

PNA errors and Operating System errors are displayed and logged in an error file. You can choose how to display PNA errors, or choose to not display PNA errors at all.

### [Error Preferences](#)

### [View Error Log](#)

### [List of PNA Errors](#)


### [SCPI Errors](#)

## Other Support topics


## Error Preferences

By default, error messages appear on the PNA screen for a brief period. You can choose to have them stay on the screen until you click an OK button, or have them not appear at all. When they stay on the screen, a Help button is available to provide further assistance.

### How to select Error Preferences

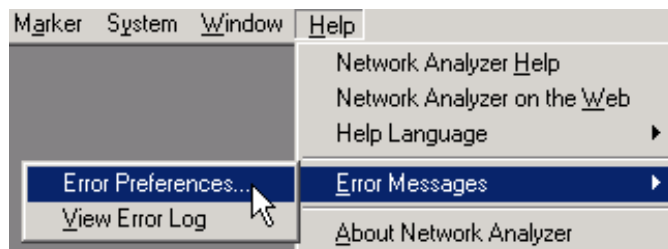

Learn more about using the [front panel interface](#)

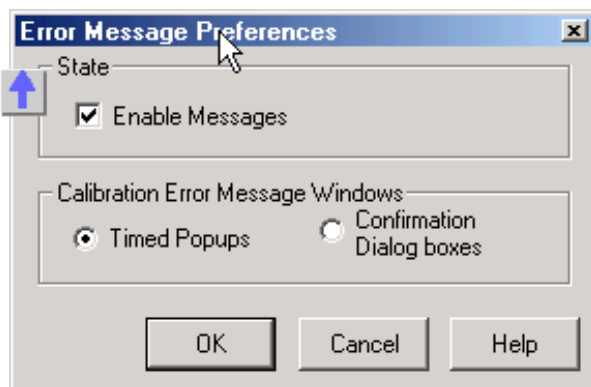



## Error Preferences dialog box help

**Enable Messages** Check to display all PNA error messages as they occur. Clear to suppress the display of PNA error messages. You can still view them in the [error log](#).

### Calibration Error Message Windows


**Timed Popups** Displays error messages on the screen for a duration of time proportional to the length of the message. You can then view the message in the [error log](#) and get further assistance.

**Confirmation Dialog boxes** Displays error messages in a standard dialog box. You then choose OK or Cancel to close the dialog box, or press Help to get further information on the error message.


## View Error Log

The PNA Error Log is a list of all events that have occurred. (Events are used in programming the PNA using COM.) PNA errors is a subset of PNA events. Only events with severity codes of ERROR are displayed on the PNA screen as they occur. From the error log, you can access further help with an error by selecting the error and clicking Help.

### How to view the Error Log

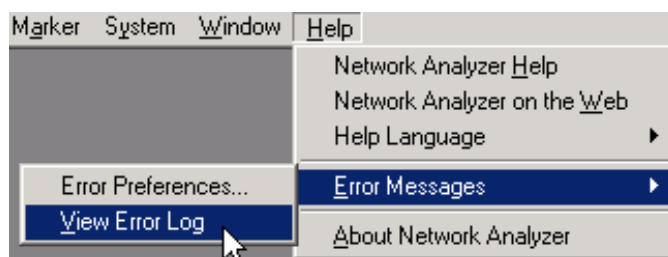

Learn more about using the [front panel interface](#)

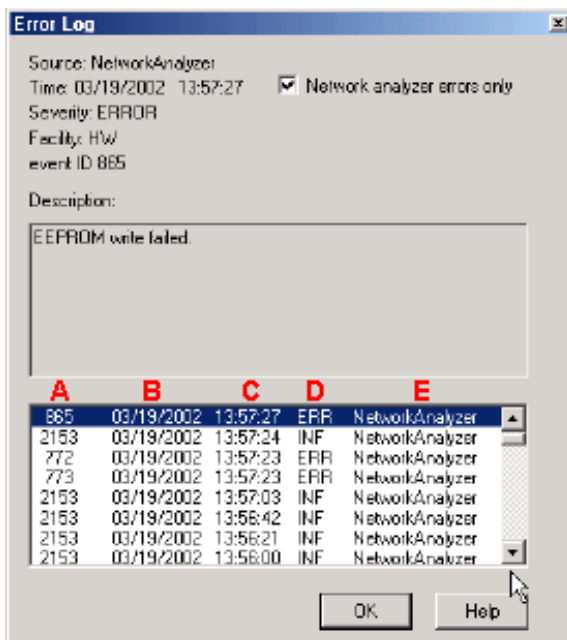

## Error Log dialog box help

**Network analyzer errors only** Select to view only PNA errors. Clear to view all errors that occur on all applications of the computer.

**Description** Error message that appears on the PNA screen.

**A - Event ID** Error message number

**B - Date** the Error occurred

**C - Time** the Error occurred

**D - Severity Code** - All events have one of the following severity codes:

- **SUC**cess - the operation completed successfully
- **IN**Formational - events that occur without impact on the measurement integrity
- **WAR**ning - events that occur with potential impact on measurement integrity
- **ERR**or - events that occur with serious impact on measurement integrity

**E - Application** in which the error occurred.

**OK** Closes the Dialog box

**Help** Provides further information on the selected Error message

To clear the Error Log:

1. From the **View** menu click **Minimize Application**
2. On the desktop, select **Start, Settings, Control Panel**
3. On the Control Panel, click **Administrative Tools**
4. On the Administrative Tools window, click **Event Viewer**
5. On the Event Viewer window, right-click **Application Log**
6. Select **Clear all Events**
7. If you want to save a file with the contents of the Event Log, click **Yes**. Otherwise, click **No**

To restore the PNA application, click on the PNA Analyzer taskbar button at the bottom of the screen

## Analyzer Accessories

---

[Goax Mechanical Calibration Kits](#)

[Waveguide Mechanical Calibration Kits](#)

[Electronic Calibration \(ECal\)](#)

[Mechanical Verification Kits](#)

[Adapter and Accessory Kits](#)

[Test Port Cables](#)

[USB Peripherals](#)

[Connector Care and Cleaning Supplies](#)

[ESD Protection](#)

### Other Support topics

For product and order information:

- Call 1-800-452-4844 (8am-8pm EST)
- Visit [www.agilent.com/find/accessories](http://www.agilent.com/find/accessories)  
Use the search function to locate information about a particular accessory or view the entire RF and Microwave Test Accessories Catalog.

Accessories are available in these connector types:

- 50 ohm Type-N
-  • 75 ohm Type-N
- 3.5 mm
- 7 mm (APC-7)
- 7-16
- 2.92 mm
- 2.4 mm
- 1.85 mm
- 1 mm

Test port cables and a calibration kit are necessary for a complete measurement system.

A verification kit is used to verify corrected system performance.

See the connector type for each PNA model

### Coax Mechanical Calibration Kits

| Model                             | Connector Type  | Frequency Upper Limit |
|-----------------------------------|-----------------|-----------------------|
| 85032B                            | Type-N (50 Ohm) | 6 GHz                 |
| 85032F                            | Type-N (50 Ohm) | 9 GHz                 |
| 85054B                            | Type-N (50 Ohm) | 18 GHz                |
| 85036E                            | Type-N (75 Ohm) | 3 GHz                 |
| 85050B                            | 7 mm            | 18 GHz                |
| 85033D                            | 3.5 mm          | 6 GHz                 |
| 85038A                            | 7-16            | 7.5 GHz               |
| 85033E                            | 3.5 mm          | 9 GHz                 |
| 85052B                            | 3.5 mm          | 26.5 GHz              |
| 85052C                            | 3.5 mm TRL      | 26.5 GHz              |
| 85056K                            | 2.92 mm         | 50 GHz                |
| 85056A                            | 2.4 mm          | 50 GHz                |
| 85058B/E<br>( <u>data-based</u> ) | 1.85 mm         | 67 GHz                |
| 85059A<br>( <u>data-based</u> )   | 1.00 mm         | 110 GHz               |

### Waveguide Mechanical Calibration Kits

| Model   | Connector Type | Frequency Range |
|---------|----------------|-----------------|
| X11644A | WR-90          | 8.2-12.4 GHz    |
| P11644A | WR-62          | 12.4-18 GHz     |
| K11644A | WR-42          | 18-26.5 GHz     |
| R11644A | WR-28          | 26.5-40 GHz     |
| Q11644A | WR-22          | 33-50 GHz       |
| U11644A | WR-19          | 40-60 GHz       |
| V11644A | WR-15          | 50-75 GHz       |

### Electronic Calibration (ECal)

| Model               | Connector Type                                                       | Frequency Range                               |
|---------------------|----------------------------------------------------------------------|-----------------------------------------------|
| <b>RF Two-Port</b>  |                                                                      |                                               |
| 85091C              | 7 mm (APC-7)                                                         | 300 kHz-9 GHz                                 |
| 85092C              | Type-N (50 ohm)<br>Port B available with 3.5 mm or 7-16 <sup>a</sup> | 300 kHz-9 GHz                                 |
| 85093C              | 3.5 mm<br>Port B available with Type-N (50 ohm) or 7-16 <sup>a</sup> | 300 kHz-9 GHz                                 |
| 85096C              | Type-N (75 ohm)                                                      | 300 kHz-3 GHz                                 |
| 85098C              | 7-16 <sup>a</sup><br>Port B available with Type-N (50 ohm) or 3.5 mm | 300 kHz-7.5 GHz                               |
| 85099C              | Type-F                                                               | 300 kHz-3 GHz                                 |
| <b>RF Four-Port</b> |                                                                      |                                               |
| N4431A Option 010   | 3.5mm (f) (four-port)                                                | 300 kHz-9 GHz<br>300 kHz-13.5 GHz (Sept 2004) |
| N4431A Option 020   | Type-N (f) (four-port)                                               | 300 kHz-9 GHz<br>300 kHz-13.5 GHz (Sept 2004) |

| <b>Microwave Two-Port</b> |                 |                                               |
|---------------------------|-----------------|-----------------------------------------------|
| N4690A                    | Type-N (50 ohm) | 10 MHz-18 GHz<br>300 kHz-18 GHz (Sept 2004)   |
| N4691A                    | 3.5 mm          | 10 MHz-26.5 GHz<br>300 kHz-18 GHz (Sept 2004) |
| N4692A                    | 2.92 mm         | 10 MHz-40 GHz                                 |
| N4693A                    | 2.4 mm          | 10 MHz-50 GHz                                 |
| N4694A                    | 1.85 mm         | 10 MHz-67 GHz                                 |
| N4696A                    | 7 mm            | 10 MHz-18 GHz                                 |

a Limits ECal module high frequency to 7.5 GHz.

### Verification Kits

| <b>Model</b> | <b>Connector Type</b> | <b>Frequency Range</b> |
|--------------|-----------------------|------------------------|
| 85055A       | Type-N (50 Ohm)       | 300 kHz-9 GHz          |
| 85053B       | 3.5 mm                | 300 kHz-26.5 GHz       |
| 85057B       | 2.4 mm                | .045-50 GHz            |
| R11645A      | WR-28                 | 26.5-40 GHz            |
| Q11645A      | WR-22                 | 33-50 GHz              |

### Adapters and Accessory Kits

| Model  | Description                                       |
|--------|---------------------------------------------------|
| 11878A | Type-N to 3.5 mm Adapter Kit                      |
| 11525A | Type-N (m) to 7 mm (APC-7)                        |
| 11853A | Type-N Accessory Kit                              |
| 11900B | 2.4 mm (f) to 2.4 mm (f)                          |
| 11900C | 2.4 mm (f) to 2.4 mm (m)                          |
| 85130G | Test Port Adapter Set, 2.4 mm (f) to 2.4 mm (m,f) |
| 11901B | 2.4 mm (f) to 3.5 mm (f)                          |
| 11901D | 2.4 mm (f) to 3.5 mm (m)                          |
| 85130F | Test Port Adapter Set, 2.4 mm (f) to 3.5 mm (m,f) |
| 11902B | 2.4 mm (f) to 7 mm (APC-7)                        |
| 11920A | 1 mm (m) to 1 mm (m)                              |
| 11920B | 1 mm (f) to 1 mm (f)                              |
| 11920C | 1 mm (m) to 1 mm (f)                              |
| 11921A | 1 mm (m) to 1.85 mm (m)                           |
| 11921B | 1 mm (f) to 1.85 mm (f)                           |
| 11921C | 1 mm (m) to 1.85 mm (f)                           |
| 11921D | 1 mm (f) to 1.85 mm (m)                           |
| 11922A | 1 mm (m) to 2.4 mm (m)                            |
| 11922B | 1 mm (f) to 2.4 mm (f)                            |
| 11922C | 1 mm (m) to 2.4 mm (f)                            |
| 11922D | 1 mm (f) to 2.4 mm (m)                            |

## Test Port Cables

| Model  | Description                                                          |
|--------|----------------------------------------------------------------------|
| N4697E | 1.85 mm (f) to 1.85 mm (rugged f) flexible (single)                  |
| N4697F | 1.85 mm (rugged f, f) to 1.85 mm (rugged m, rugged f) flexible (set) |
| N6315A | Type-N (m) to Type-N (f), 16 in. (single)                            |
| N6314A | Type-N (m) to Type-N (m), 24 in. (single)                            |
| 85133D | 2.4 mm (f) to 2.4 mm (m,f) semi-rigid (set)                          |
| 85133F | 2.4 mm (f) to 2.4 mm (m,f) flexible (set)                            |
| 85134D | 2.4 mm (f) to 3.5 mm (m,f) semi-rigid (set)                          |
| 85134F | 2.4 mm (f) to 3.5 mm (m,f) flexible (set)                            |

### USB Peripherals

| Model  | Description                                                                                                                          |
|--------|--------------------------------------------------------------------------------------------------------------------------------------|
| N4688A | <b>CD RW drive</b> - with USB cable.                                                                                                 |
| N4689A | <b>USB 4-port hub</b> - for connecting additional USB peripherals.                                                                   |
| 82357A | <b>USB/GPIB Interface</b> - for controlling GPIB devices through USB. Learn more about <a href="#">using the 82357A with the PNA</a> |

### Connector Care and Cleaning Supplies

| Part Number | Description                      |
|-------------|----------------------------------|
| 9301-1243   | Lint-Free Swabs (small), 100 ct. |
| 8500-5344   | IPA 99.5% alcohol, 30 ml. bottle |
| 8500-6659   | Compressed Air, 235 ml. can      |
| 5021-7607   | Type-N Contact Removal Tool      |
| 1401-0225   | Standard End-Cap, Type-N (m)     |
| 1401-0248   | ESD Safe End-Cap, Type-N (m)     |
| 1401-0225   | Standard End-Cap, Type-N (f)     |



|           |                              |
|-----------|------------------------------|
| 1401-0247 | ESD Safe End-Cap, Type-N (f) |
|-----------|------------------------------|

### ESD Supplies

| Part Number | Description                                                       |
|-------------|-------------------------------------------------------------------|
| 9300-1367   | Adjustable antistatic wrist strap                                 |
| 9300-0980   | Antistatic wrist strap grounding cord (5 foot)                    |
| 9300-0797   | Static control table mat (2 foot x 4 foot) with earth ground wire |
| 9300-1126   | ESD heel strap                                                    |

## 82357A USB / GPIB Interface

---

The Agilent 82357A is an adapter that creates a GPIB Interface from one of your unused PNA USB ports.

### [Applications](#)

### [Installing](#)

### [Configuring](#)

### [Connecting](#)

### [Communicating with other Equipment](#)

---

## Applications

The 82357A can be used for the following PNA applications:

- **Frequency Converter Application** - The 82357A is included with the Frequency Converter Application ([option 083](#)). External sources **MUST** be connected to this Interface if controlling the PNA using an external PC. See [connecting diagram](#) below. To learn more, see [Configure an external LO source](#).

---

**Note:** If the PNA is [hibernated](#) during an FCA measurement involving an external source under FCA control, and then the PNA is restarted, a VISA error message will appear stating "VI\_ERROR\_INV\_OBJECT." To correct this problem, the 82357 USB/GPIB interface must be reinitialized after hibernation. This is done by clicking on the Accept button in the interface initialization dialog box. The green READY light on the interface will illuminate.

---


- **PNA Controller** - The 82357A can be used by the PNA to control other GPIB devices. This frees the default GPIB interface to perform other GPIB operations, such as control the PNA from an external PC.
- **Source Power Cal** - The 82357A can be used to run a source power calibration.

## Installing the 82357A USB/GPIB Interface

1. [Download and install firmware](#) PNA revision 3.0 or greater. To check the revision of your PNA firmware, click **Help** then **About Network Analyzer**.
2. Upgrade to the latest Agilent IO libraries from the CDROM that was shipped with the 82357A. If not available, download them from [www.Agilent.com](http://www.Agilent.com) (search for **82357A**)

## Configure the 82357A USB/GPIB Interface

When the 82357A is connected to the PNA USB, the following dialog box appears:

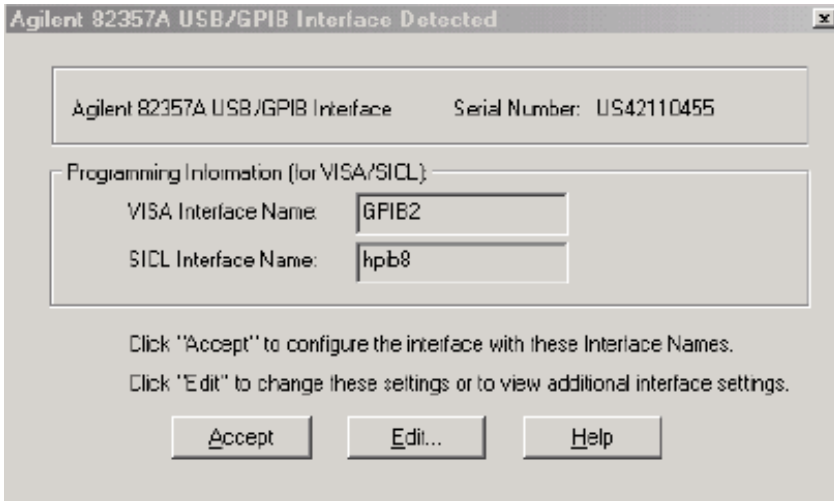


Normally, you do NOT need to edit these settings. The 82357A USB/GPIB Interface is configured automatically as the next unused VISA interface. This is usually **GPIB2** unless you have already configured it for another purpose.

If the VISA Interface Name appears as GPIB0 or GPIB1, these Interfaces must be returned to their default settings for the 82357A to work properly with the PNA. See Configure for VISA / SICL to learn how.

### Connecting the 82357A USB/GPIB Interface

The following diagram illustrates how to connect GPIB test equipment using the USB/GPIB Interface.

- Plug the USB/GPIB Interface into any unused PNA USB port.
- The default GPIB Interface and USB/GPIB Interface should never be connected together.

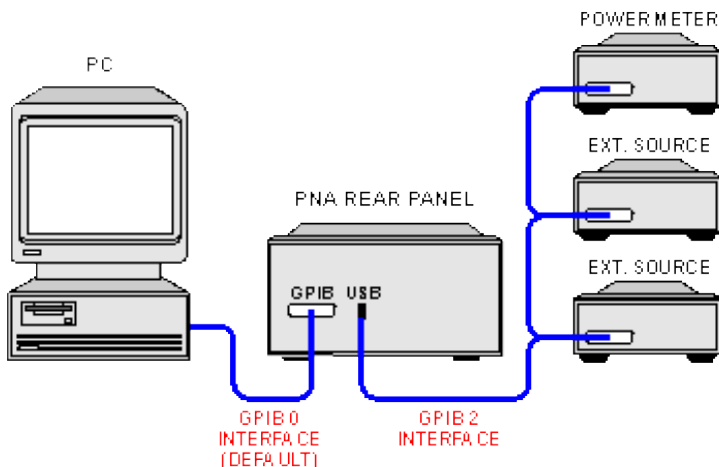

### Communicating with Equipment Connected to the USB/GPIB Interface

- The Frequency Converter Application will automatically find and communicate with test equipment that is connected to the USB/GPIB Interface.
- Source power calibration will automatically find and communicate with the power meter that is connected to the USB/GPIB Interface.
- To control other devices through your own program using the 82357A, you must include the new GPIB Interface number when addressing the devices.



## Firmware Upgrade

---

PNA firmware upgrades are available to you at no cost in a self-extracting Install Shield file. The upgrade includes the PNA application, Online help, and Service utilities. Note: The file is at least 45 MB.

The following options are available for you to upgrade your PNA application:

- [Auto-Check](#) and [AgileUpdate](#) If your PNA is connected to the Internet, these utilities will automatically check for, download, and install, the new firmware and associated files when the PNA application is started. You will be prompted before this occurs.
- [Website Access](#) If your PNA is NOT connected to the Internet, but you have a PC that is, you can download the PNA firmware and associated files to a storage medium.

### Other Support Topics

#### Auto-Check

With Internet access to your PNA, Auto-Check automatically and regularly checks the Internet for new PNA firmware revisions. If a new revision is found, a notification message prompts you to run the [AgileUpdate](#) utility, which then performs the actual download.

Without Internet access to your PNA, Auto-Check provides a reminder prompt at the selected intervals.


Auto-Check is run only when the PNA application is started. Once the PNA application is running, it will not check for updates again until it is restarted.

When Auto-Check runs, it checks the following conditions:

- Is there an active connection to the Internet?
- Is the Auto-Check utility enabled?
- Is it time to check for new firmware?
- Does new firmware exist?

 If all of these conditions are true, Auto-Check shows the following dialog box.

If all of these conditions are NOT true, or to change these settings at any time, click **System, Service**, then **AgileUpdate**. From within AgileUpdate, click **AutoCheck**. These preferences are stored in the PNA registry. Future firmware upgrades will not change these settings.

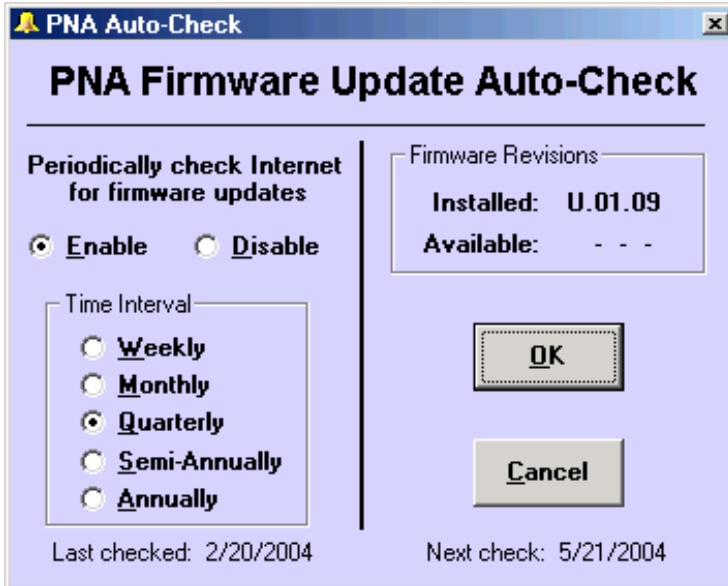

### PNA Auto-Check dialog box help

**Enable** When the PNA application is started, Auto-Check will search the PNA website for firmware updates at the selected time interval.

**Disable** When the PNA application is started, Auto-Check will NOT search the PNA website for firmware updates.

**Time Interval** Select the time interval Auto-Check is to search for firmware updates.

**OK** Starts AgileUpdate.


**Cancel** No further action is taken until the selected time interval has elapsed.

## AgileUpdate

**Note:** You must have administrative privileges on the analyzer to run this utility. See [Set Up Analyzer Users](#).

In most cases, the following steps are sufficient to download and install the newest version of PNA firmware:

1. Connect the PNA to the Internet. A LAN connection is recommended because a firmware download can take many hours using a modem.
2. In the **System** menu, click **Service**, then **AgileUpdate**.
3. Click **Check for Updates**.
4. If updates exist, click **Download & Install**.

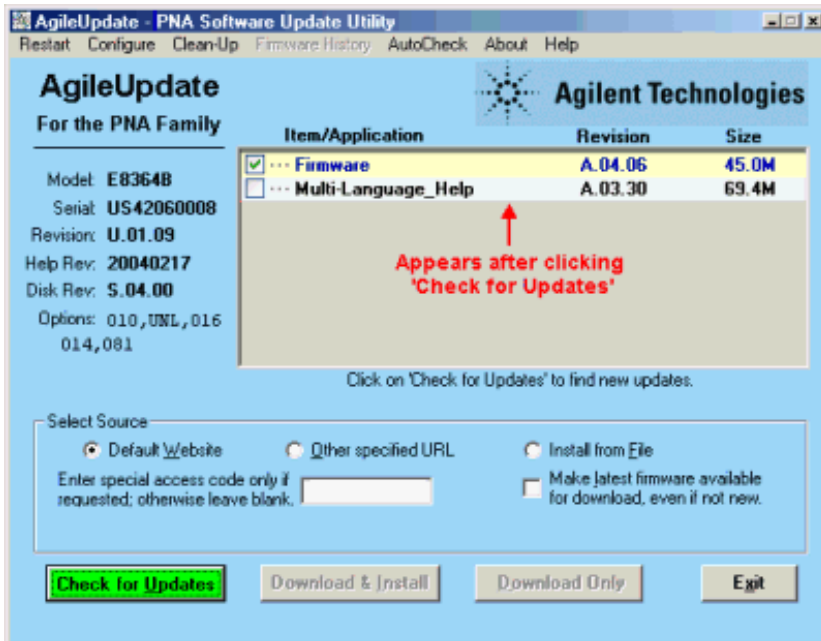

## AgileUpdate dialog box help

**Note:** Your privacy is important to Agilent. AgileUpdate does NOT send ANY information from the PNA to the server. It only downloads from the server to the PNA.

**Restart** Click to restart from the beginning.

**Configure** Click to launch the [Configure dialog box](#).

**Clean-up** Click to delete all but the two most recent install shield packages from the PNA hard drive.

**Firmware History** Available after clicking **Check for Updates**.

**Auto-Check** Launches the [Auto-Check](#) dialog box.

**Item / Application** Lists the items available for download at the firmware website.

- Click on items with **i** to read more information about the download.
- Items in RED should be downloaded and installed individually.
- Multi-language help includes all help files except English.

**Note:** The firmware includes the help file. Therefore, only the firmware checkbox will be selected if a new version for both the firmware and the help file are available.

### Select Source

**Default Website** The Agilent site that contains upgrade FW.

**Other Specified URL** Click if you were instructed to get firmware from a different website.

**Install from File** Click if you have already downloaded the InstallShield package and want AgileUpdate to install it for you.

**Special Access Code...** Type in the code if you were given one from Agilent Technical Support. Otherwise, leave blank.


**Make Latest Firmware Available...** Select this checkbox if you want to download the latest firmware, even if it is not new.

**Check for Updates** Click to look for firmware updates at the Agilent website. If there are newer versions, the

files will be listed.

**Download and Install** When updates are found, this selection becomes available. Some files may be pre-checked. Be sure the corresponding boxes are checked for the files you want to download. Then click to download and install the update.

**Download Only** Click to download the files to the analyzer hard disk and install the files at a later time. At that time, click **Install from File**.

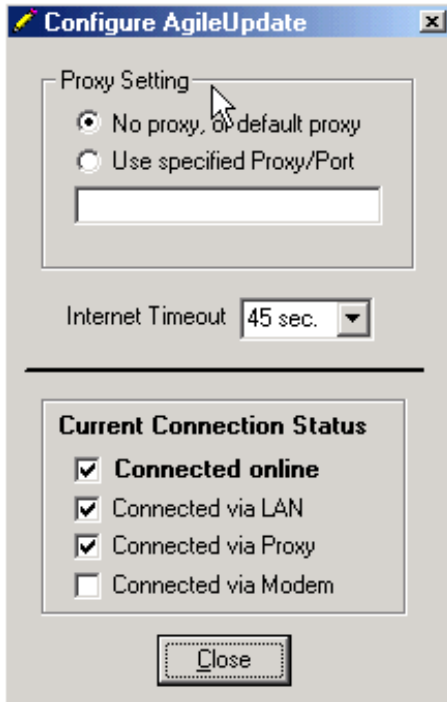

### Configuration dialog box help

**Note:** If AgileUpdate will not connect, try to access ANY Internet website. Contact your local IT department if necessary.

#### Proxy Setting

**No Proxy or Default Proxy** Click if you use a LAN connection. AgileUpdate will automatically use the proxy specified in Internet Explorer.

**Use specified Proxy / Port** Click to enter the proxy name and port. The format is: proxyName:portNumber. (The proxy port number is typically 8088).

**Internet timeout** If you are using an automatic dial-up Internet connection you may need to increase the timeout.

**Current Connection Status** Shows the current status of the PNA connection to the Internet.

**Note:** These settings are NOT saved; they must be re-entered each time AgileUpdate is run.

## Agilent Website Access

If you cannot access the Internet directly with your analyzer, you can use an external PC with Internet access to download the file from the Agilent website. You can then transfer the file from your PC to your analyzer over a LAN or other means.



1. Connect to the PNA web page at <http://www.agilent.com/find/PNA>.
2. Follow the links, or search for the "PNA firmware" download page.
3. Click on the firmware to be downloaded.
4. Save the program to disk (hard drive of your PC).
5. Transfer the file from your PC to your PNA using LAN, CD, or USB Pen drive.
6. Double-click the file on the PNA.

---

**Warning:** You can save the upgrade file to your PC, but do not attempt to install the PNA application on your PC. It will alter system settings and can result in system crashes.

---

## PNA Configurations and Options

Included with each PNA is a mouse, keyboard. This topic presents standard PNA models and the available options and upgrades.

### [PNA Models](#)

#### [PNA L Series](#)

#### [Microwave Models](#)

#### [RF Models](#)

#### [mmWave Model](#)

### [Options and Upgrade Kits](#)

### [Warranty Period](#)

To view the options that are installed on your analyzer, click **Help** then **About Network Analyzer**


A documentation CD-ROM is no longer included in each PNA shipment (Feb.05).

### [Other Support Topics](#)

## PNA-L Series Model N5230A

Click the **Option number** to see the block diagram.

Click the **Connector type** to see the connector specifications.

| Option                                                                                                  | Frequency Range    | Test Ports | Connector                   | Reference Receivers | Test Set <sup>1</sup>     |
|---------------------------------------------------------------------------------------------------------|--------------------|------------|-----------------------------|---------------------|---------------------------|
| <a href="#">020</a>                                                                                     | 300 KHz* to 6 GHz  | 2          | <a href="#">3.5 mm</a> Male | 2                   | Standard                  |
|  <a href="#">025</a> | 300 KHz* to 6 GHz  | 2          | <a href="#">3.5 mm</a> Male | 2                   | Configurable              |
| <a href="#">120</a>                                                                                     | 300 KHz* to 13 GHz | 2          | <a href="#">3.5 mm</a> Male | 2                   | Standard                  |
| <a href="#">125</a>                                                                                     | 300 KHz* to 13 GHz | 2          | <a href="#">3.5 mm</a> Male | 2                   | Configurable              |
| <a href="#">220</a>                                                                                     | 10 MHz* to 20 GHz  | 2          | <a href="#">3.5 mm</a> Male | 2                   | Standard                  |
| <a href="#">225</a>                                                                                     | 10 MHz* to 20 GHz  | 2          | <a href="#">3.5 mm</a> Male | 2                   | Configurable              |
| <a href="#">240</a>                                                                                     | 300 KHz* to 20 GHz | 4          | <a href="#">3.5 mm</a> Male | 1                   | Standard                  |
| <a href="#">245</a>                                                                                     | 300 KHz* to 20 GHz | 4          | <a href="#">3.5 mm</a> Male | 1                   | Configurable <sup>2</sup> |
| <a href="#">420</a>                                                                                     | 10 MHz* to 40 GHz  | 2          | <a href="#">2.4 mm</a> Male | 2                   | Standard                  |
| <a href="#">425</a>                                                                                     | 10 MHz* to 40 GHz  | 2          | <a href="#">2.4 mm</a> Male | 2                   | Configurable              |

|            |                   |          |                    |          |                     |
|------------|-------------------|----------|--------------------|----------|---------------------|
| <b>520</b> | 10 MHz* to 50 GHz | <b>2</b> | <u>2.4 mm</u> Male | <b>2</b> | <b>Standard</b>     |
| <b>525</b> | 10 MHz* to 50 GHz | <b>2</b> | <u>2.4 mm</u> Male | <b>2</b> | <b>Configurable</b> |

\* Typical specs apply

**1 Test Set**

**Standard** NO Configurable Test Set.

**Configurable** - Adds six front panel access loops and two 50 dB step attenuators.

**2 Configurable** - Adds nine front panel access loops and one 60 db step attenuator.

**Microwave Standard Models** (see options)

Click the **PNA model** to see the block diagram.

Click the **Connector type** to see the connector specifications.

| <b>PNA Model</b> | <b>Frequency Range</b>                     | <b>Port</b> | <b>Connector Type</b> | <b>Reference Receivers</b> | <b>Front Panel Jumpers</b> |
|------------------|--------------------------------------------|-------------|-----------------------|----------------------------|----------------------------|
| <u>E8361A</u>    | 10 MHz* to 67 GHz<br>(tunable to 70 GHz)** | <b>2</b>    | <u>1.85 mm</u> Male   | <b>2</b>                   | <b>0</b>                   |
| <b>E8362A</b>    | 45 MHz to 20 GHz                           | <b>2</b>    | <u>3.5 mm</u> Male    | <b>2</b>                   | <b>0</b>                   |
| <b>E8363A</b>    | 45 MHz to 40 GHz                           | <b>2</b>    | <u>2.4 mm</u> Male    | <b>2</b>                   | <b>0</b>                   |
| <b>E8364A</b>    | 45 MHz to 50 GHz                           | <b>2</b>    | <u>2.4 mm</u> Male    | <b>2</b>                   | <b>0</b>                   |
| <u>E8362B</u>    | 10 MHz* to 20 GHz                          | <b>2</b>    | <u>3.5 mm</u> Male    | <b>2</b>                   | <b>0</b>                   |
| <u>E8363B</u>    | 10 MHz* to 40 GHz                          | <b>2</b>    | <u>2.4 mm</u> Male    | <b>2</b>                   | <b>0</b>                   |
| <u>E8364B</u>    | 10 MHz* to 50 GHz                          | <b>2</b>    | <u>2.4 mm</u> Male    | <b>2</b>                   | <b>0</b>                   |

**Legend**

**No longer produced**

\* Typical specs apply from 10 to 45 MHz

\*\* Typical specs apply from 67 to 70 GHz

**RF Standard Models** (see options)

Click the **PNA model** to see the block diagram.

Click the **Connector type** to see the connector specifications.

| PNA Model              | Frequency Range  | Ports | Connector Type                | Reference Receivers | Front Panel Jumpers |
|------------------------|------------------|-------|-------------------------------|---------------------|---------------------|
| <a href="#">E8356A</a> | 300 kHz to 3 GHz | 2     | <a href="#">Type-N</a> Female | 2                   | 4                   |
| <a href="#">E8357A</a> | 300 kHz to 6 GHz | 2     | <a href="#">Type-N</a> Female | 2                   | 4                   |
| <a href="#">E8358A</a> | 300 kHz to 9 GHz | 2     | <a href="#">Type-N</a> Female | 2                   | 4                   |
| <a href="#">E8801A</a> | 300 kHz to 3 GHz | 2     | <a href="#">Type-N</a> Female | 1                   | 0                   |
| <a href="#">E8802A</a> | 300 kHz to 6 GHz | 2     | <a href="#">Type-N</a> Female | 1                   | 0                   |
| <a href="#">E8803A</a> | 300 kHz to 9 GHz | 2     | <a href="#">Type-N</a> Female | 1                   | 0                   |
| <a href="#">N3381A</a> | 300 kHz to 3 GHz | 3     | <a href="#">Type-N</a> Female | 1                   | 0                   |
| <a href="#">N3382A</a> | 300 kHz to 6 GHz | 3     | <a href="#">Type-N</a> Female | 1                   | 0                   |
| <a href="#">N3383A</a> | 300 kHz to 9 GHz | 3     | <a href="#">Type-N</a> Female | 1                   | 0                   |

### Millimeter Wave PNA

| PNA Model     | Frequency Range    | Ports | Connector Type | Reference Receivers | Front Panel jumpers |
|---------------|--------------------|-------|----------------|---------------------|---------------------|
| <b>N5250A</b> | 10 MHz* to 110 GHz | 2     | 1.0 mm         | 2                   | <b>N5260A</b>       |

\* [Typical specs](#) apply from 10 to 45 MHz  
 Test heads to 325 GHz are also available  
 Upgrade your existing E836xB with the following:

- [H11 option](#)
- N5260A Test Set
- Millimeter-Wave VNA Frequency Extension Modules from Oleson Microwave Labs Extension Modules

### Options and Upgrade Kits

The following options are installed at the time of purchase, and some are also available after the initial purchase of a PNA. To order an upgrade, contact your [Agilent representative](#).

| Option | Supported Models | Description |
|--------|------------------|-------------|
|--------|------------------|-------------|

|            |                                                                                |                                                                                                                                                                                                                                                                                                                                                 |
|------------|--------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>006</b> | E8356A<br>E8801A<br>N3381A                                                     | <b>Upgrade to 6 GHz frequency range.</b><br>Adds 6 GHz operation. Includes installation at an Agilent service center. Instrument calibration (required after frequency upgrade) is available for an additional fee.                                                                                                                             |
| <b>009</b> | E8356/7A<br>E8801/2A<br>N3381/2A                                               | <b>Upgrade to 9 GHz frequency range.</b><br>Adds 9 GHz operation. Includes installation at an Agilent service center. Instrument calibration (required after frequency upgrade) is available for an additional fee.                                                                                                                             |
| <b>010</b> | All                                                                            | <b>Time-domain</b><br>Adds time-domain capability to analyzer. The serial number of the analyzer must be specified when ordering this kit. Software upgrade.<br><a href="#">Learn more</a>                                                                                                                                                      |
| <b>014</b> | E8801/ 02/ 03A<br>N3381/ 82/ 83A<br>E8361A<br>E8362/ 63/ 64A<br>E8362/ 63/ 64B | <b>Configurable test set</b><br>Adds front panel access to the source output and coupler input on test ports 1 and 2. Adds front panel access directly to all receivers, including the reference receiver.<br>Upgrade includes installation at an Agilent service center.<br><a href="#">See the PNA block diagram.</a>                         |
| <b>015</b> | E8356/ 57/ 58A                                                                 | <b>Configurable test set</b><br>Adds front panel access to the source output and coupler input on test ports 1 and 2.<br>Adds 35 dB step attenuators between the couplers and receivers.<br>Upgrade includes installation at an Agilent service center.<br><a href="#">See the PNA block diagram</a>                                            |
| <b>016</b> | E8361A<br>E8362/ 63/ 64B                                                       | <b>Receiver Step Attenuators</b><br>Adds two step attenuators. (E8361A adds 50 dB step attenuators with 10 dB resolution; all other PNA models add 35 dB step attenuators with 5 dB resolution.) Each attenuator is inserted between a test port and its corresponding receiver. Requires option UNL.                                           |
| <b>022</b> | E8361A<br>E8362/ 63/ 64B                                                       | <b>Extended Memory</b><br>Adds more RAM for a total of 512MB. <a href="#">Learn more about PNA RAM</a>                                                                                                                                                                                                                                          |
| <b>080</b> | E8361A<br>E8362/ 63/ 64B<br>N5230A                                             | <b>Frequency Offset</b><br>Enables you to set the PNA source independently from where the receivers are tuned. This capability is important for measuring mixers, converters, and amplifiers. To control the additional hardware, a basic user interface, SCPI, and COM commands are provided. Requires option 014 or Active test set (N5230A). |

|            |                                  |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
|------------|----------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>081</b> | E8361A<br>E8362/ 63/ 64B         | <b>Reference Switch</b><br>Adds an internal solid state switch in the R1 reference path for controlling an external reference mixer. Requires option 014 and opt 080<br>See a <a href="#">block diagram of reference switch</a> .                                                                                                                                                                                                                                                                                                      |
| <b>083</b> | E8361A<br>E8362B/ 63B/ 64B       | <b>Frequency Converter Measurement Application</b><br>Provides an intuitive user-interface for making extremely accurate conversion loss and absolute group delay measurements on mixers and converters. Exceptional amplitude and phase accuracy is achieved through two new calibration techniques: match-corrected power meter calibration and vector mixer calibration. The application also provides automatic control of all of Agilent's major signal sources. Requires option 014, 080, and 081.<br><a href="#">Learn more</a> |
| <b>098</b> | E8356/ 57/ 58A                   | <b>CPU board upgrade</b><br>Replaces the 266 MHz CPU board with a 500 MHz CPU board.<br>Upgrade includes installation at an Agilent service center. Learn how to check your <a href="#">PNA CPU speed</a> .                                                                                                                                                                                                                                                                                                                            |
| <b>1E1</b> | E8801/ 02/ 03A<br>N3381/ 82/ 83A | <b>70 dB step attenuator</b><br>Adds a single 70 dB step attenuator that is switched between the source and each output port to extend the output power to -85 dBm. <b>Note:</b> Two 70 dB step attenuators are standard equipment with PNA models E8356/ 57/ 58A.<br>Upgrade includes installation at an Agilent service center.                                                                                                                                                                                                      |
| <b>1E5</b> | E8801/ 02/ 03A<br>N3381/ 82/ 83A | <b>High stability 10 MHz time base</b><br>Replaces 10 ppm time base with a 1 ppm time base. High stability time base is standard with PNA models E8356/ 57/ 58A and E8362/ 63/ 64B.                                                                                                                                                                                                                                                                                                                                                    |
| <b>H08</b> | E8361A<br>E8362B/ 63B/ 64B       | <b>Pulsed Measurement Application</b><br>Provides the Pulsed Application for average pulse and point-in-pulse measurements. Requires options H11, UNL, 014, 080, and 081.<br><a href="#">Learn more</a>                                                                                                                                                                                                                                                                                                                                |
| <b>H11</b> | E8361A<br>E8362B/ 63B/ 64B       | <b>IF Access</b><br>Provides rear panel access to the PNA IF paths for: <ul style="list-style-type: none"> <li>• Extended frequency coverage to 325 GHz</li> <li>• Pulsed measurement capability</li> <li>• Advanced antenna measurements</li> </ul> Requires options UNL, 014, 080, and 081.<br><a href="#">Learn more</a>                                                                                                                                                                                                            |

|            |                                            |                                                                                                                                                                                                                                                                                                                                                                                                                                            |
|------------|--------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>UNL</b> | E8361A<br>E8362/ 63/ 64A<br>E8362/ 63/ 64B | <p><b>Extended power range and bias tees</b></p> <p>Adds two step attenuators and two bias tees. (E8361A adds 50 dB step attenuators; E8362/ 63/ 64A/B adds 60 dB step attenuators. All attenuators have a 10 dB resolution.) A step attenuator and bias-tee set is inserted between the source and test port 1 and another set between the source and test port 2.</p> <p>Upgrade includes installation at an Agilent service center.</p> |
|------------|--------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

### Certification Options

| Option     | Supported Models                     | Description                                                                                                                                                                                                                                                                            |
|------------|--------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>1A7</b> | E8361A<br>E8362B/ 63B/ 64B<br>N5250A | Complete set of measurement data which was acquired from testing your PNA to published specifications. Includes calibration label, calibration certificate, and data report. Conforms to ISO 9001.                                                                                     |
| <b>UK6</b> | E8361A<br>E8362B/ 63B/ 64B<br>N5250A | Complete set of measurement data which was acquired from testing your PNA to published specifications. Includes calibration label, ISO 17025 calibration certificate, data report, measurement uncertainties and guard bands on all specifications. Conforms to ISO17025 and ISO 9001. |

### Documentation and Localization Options

|                                                                                                                                                                                                 |
|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b>                                                                                                                                                                              |
| Printed versions of PNA Help in pdf format are available at Agilent.com. (Apr.2005)                                                                                                             |
| A documentation CD-ROM is no longer included with each PNA shipment (Feb.2005).                                                                                                                 |
| To download a service guide for your PNA, or the latest version of PNA Help, visit <a href="http://www.agilent.com">http://www.agilent.com</a> , search for your PNA model, then click Library. |

### PNA Warranty Period

The actual warranty on your instrument depends on the date it was ordered as well as whether or not any warranty options were purchased at that time. To determine the exact warranty on your instrument, contact [Agilent Technologies](#) with the model and serial number of your instrument.

For online information about Agilent's service and support products visit: [www.agilent.com/find/tm\\_services](http://www.agilent.com/find/tm_services)

## Option Enable Utility

---

The Option Enable utility allows you to perform the following activities.

- Enable or remove software options and some hardware options.
- Recover option data if the hard drive or other data-containing assembly is replaced.
- Input or change a serial number.

### Keywords

### Running the Program

### Removing an Option

### Installing an Option

### Repairing and Recovering Option Data

### Installing or Changing the Serial Number

## Keywords

To add certain options, you need a keyword that is provided by Agilent. There are two types of keywords:

- **Option Keywords** to add a software option.
- **Model Keywords** that may be required if you replace multiple assemblies.

## Temporary and Permanent Options

Any software option can also be installed on a temporary basis for a specified amount of time. This allows you to evaluate a specific feature or capability at no cost.

If the license key provided by Agilent has an expiration date, you must select the "temporary" option and enter the expiration date exactly as stated in the license statement. If you decide to make this option permanent, Agilent will provide a new keyword that converts the option to permanent status.



For either permanent or temporary software options, a provided keyword must be entered.

## Running the Program

1. In the analyzer **System** menu, point to **Service**, and click **Option Enable**.
2. The first screen will display the model number, serial number, and all installed options. To enable or remove an option, select it from the drop-down list of available options.
  - If the desired option is not listed, select the last choice in the list, labeled **Enter Unlisted Option**. Next, enter the 3-character option name and click **Enter**

If a software option was chosen, the following occurs.

- The **Remove** button will be enabled.



- The keyword entry area becomes visible.
- The permanent/temporary selection is enabled.

If a hardware option is selected, the following occurs.

- With the hardware option already installed, the **Remove** button is enabled.
- With the hardware option not installed, the **Enable** button is enabled.

## Removing an Option

1. To remove an option, click **Remove**.
2. After the option is removed, restart the network analyzer application for the changes to take effect.

---

**Note:** Removal of a licensed option (such as Option 010, Time Domain) will permanently remove the license keyword. If this option **may** be needed in the future, then record the license keyword before removing the option. Do this by copying the file “gen.lic” to another location (such as a floppy disk), or print it using notepad. The file, located at “C:\Program Files\Agilent\Network Analyzer” contains all the information needed to recreate the license.

---

## Installing an Option

1. If the keyword entry area is visible, enter a keyword. (The keyword is not case sensitive.)
2. Click **Enable**.
3. After the option is installed, restart the network analyzer application for the changes to take effect.

## Repairing and Recovering Option Data

Use this part of the Option Enable Utility in the following situations:

- If the hard drive is replaced
- If the frequency reference assembly is replaced

This routine rebuilds the option information contained on the hard drive and frequency reference assembly (primary and backup).

1. Select **Repair** from the **Option Enable** menu bar.

---

**Note:** If you are unsure if this routine needs to be done, run it; no harm will result.

---

2. The model and serial number are displayed, along with four check boxes.
3. Select the boxes that apply.
4. Click **Begin Repair**. The routine checks all data files and performs any needed repairs. You may be asked to verify certain information and processes.
5. If the routine finds that the model number is incorrect or invalid, you will be asked to select the correct model number.

- Along with this model number, a model keyword will be required. If this is not labeled on the analyzer, or is not otherwise known, contact Agilent
  - After you have entered the requested data, click **Change Model**. This process takes about 30 seconds.
6. When done, click **Exit Repair**.
  7. If you do not need to install any other options, click **Exit**.

## Installing or Changing the Serial Number

It may be necessary to install or change a serial number if certain assemblies are replaced.

1. To change the serial number, select **Change Serial** from the **Option Enable** menu bar. The current serial number will be displayed. If no serial number has previously been entered, the word "NONE" will be displayed.
2. Type the new serial number into the space provided, and click **Change Serial**. (The serial number is not case sensitive.)

---

**Note:** Use extreme care when entering the serial number; only one entry chance is allowed!

---

3. To change an incorrect serial number, a clear-code password is required. Contact Agilent to obtain this clear code and have the existing serial number available. Enter the clear code in the space provided, along with the new serial number, then click **Change Serial**.

## Other Resources

---

The following network analysis resources are also available.

### [Document Resources](#)

### [Third Party Resources](#)

### [Other Support Topics](#)

## Document Resources


### Application Notes

You can access a number of the following application notes from the analyzer.

1. In the **Help** menu, click **Product Overview**.
2. The Product Overview starts with an introduction. To immediately move through this, click **Main Menu**.
3. In the main menu click **Literature**, and then any literature title to view the document.

You can also access all of the following application and product notes at this URL:

<http://www.agilent.com/find/PNA>

- Application Development with the Agilent PNA Series of Network Analyzers, (literature number 5980-2666ENUS).
- Understanding and Improving Network Analyzer Dynamic Range, Agilent Application Note 1363-1 (literature number 5980-2778EN).
- *The "Need for Speed"* in Component Manufacturing Test, (literature number 5980-2783EN).
- Generate Component Data Sheets with Agilent's BenchLinkXL, (literature number 5980-2781EN).
-  Connectivity Advances in a LAN-enabled Instrument, (literature number 5980-2782EN).
- De-embedding and Embedding S-Parameter Networks Using the PNA Series Network Analyzer, Agilent Application Note 1364-1 (literature number 5980-2784EN).
- Advanced Filter Tuning Using Time Domain, Agilent Application Note 1287-10 (literature number 5980-2785EN).
- Understanding the Fundamental Principles of Vector Network Analysis, Agilent Application Note 1287-1 (literature number 5965-7707E).
- Exploring the Architectures of Network Analyzers, Agilent Application Note 1287-2 (literature number 5965-7708E).
- Applying Error Correction to Network Analyzer Measurements, Agilent Application Note 1287-3 (literature number 5965-7709E).
- Network Analyzer Measurements: Filter and Amplifier Examples, Agilent Application Note 1287-4 (Agilent literature number 5965-7710E).

- Improving Throughput in Network Analyzer Applications, Agilent Application Note 1287-5 (literature number 5966-3317E)
- Using a Network Analyzer to Characterize High-Power Components, Agilent Application Note 1287-6 (literature number 5966-3319E)
- Simplified Filter Tuning Using Time-Domain Analysis, Agilent Application Note 1287-8 (literature number 5968-5328E).
- In-Fixture Measurements Using Vector Network Analysis, Agilent Application Note 1287-9 (literature number 5968-5329E).
- 8 Hints for Making Better Network Analyzer Measurements, Agilent Application Note AN 1291-1 (literature number 5965-8166E)
- Specifying Calibration Standards for the Agilent 8510 Network Analyzer, Agilent Product Note 8510-5A, (literature number 5956-4352, or Agilent part number 08510-90352, February 1988).
- In-Fixture Microstrip Device Measurements Using TRL\* Calibration, Agilent Product Note 8720-2, (literature number 5091-1943E, August 1991).

### Third-Party Resources

For information about test fixtures and part handlers, contact:

**Inter-Continental Microwave**  
 1515 Wyatt Drive  
 Santa Clara, CA 95054-1524 USA  
 Telephone: (408) 727-1596  
 Fax: (408) 727-0105  
 Web site: [www.icmicrowave.com](http://www.icmicrowave.com)  
 E-mail: [icmfixture@aol.com](mailto:icmfixture@aol.com)

For information about probing equipment and accessories, contact:

**Cascade Microtech, Inc.**  
 2430 NW 206th Avenue  
 Beaverton, OR 97006 USA  
 Telephone: (503) 601-1000  
 Fax: (503) 601-1002  
 Web site: [www.cascademicrotech.com](http://www.cascademicrotech.com)  
 E-mail: [sales@cmicro.com](mailto:sales@cmicro.com)

## SCPI Errors

---

### Standard SCPI Errors

-100 to -200 Command Errors

-200 to -299 Execution Errors

-300 to -399 SCPI Specified Device-Specific Errors

-400 to -800 Query and System Errors

### PNA specific Errors


---

Note: See also PNA Errors

---

#### **-100 to -200 Command Errors**

A command error indicates that the test set's GPIB parser has detected an IEEE 488.2 syntax error. When one of these errors is generated, the command error bit in the event status register is set.

|                                                                                     |                       |                                                                                                                                                                                             |
|-------------------------------------------------------------------------------------|-----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -100                                                                                | std_command           | Command - This event bit (Bit 5) indicates a syntax error, or a semantic error, or a GET command was entered, see IEEE 488.2, 11.5.1.1.4.                                                   |
| -101                                                                                | std_invalidChar       | Invalid character - Indicates a syntactic elements contains a character which is invalid for that type.                                                                                     |
| -102                                                                                | std_syntax            | Syntax - Indicates that an unrecognized command or data type was encountered. For example, a string was received when the device does not accept strings.                                   |
| -103                                                                                | std_invalidSeparator  | Invalid separator - The parser was expecting a separator and encountered an illegal character. For example, the semicolon was omitted after a program message unit.                         |
| -104                                                                                | std_wrongParamType    | Data type -The parser recognized a data element different than one allowed. For example, numeric or string data was expected but block data was encountered.                                |
| -105                                                                                | std_GETNotAllowed     | GET not allowed - Indicates a Group Execute Trigger was received within a program message. Correct the program so that the GET does not occur within the program code.                      |
|  | std_tooManyParameters | Parameter not allowed - Indicates that more parameters were received than expected for the header. For example, *ESE common command only accepts one parameter, so *ESE 0,1 is not allowed. |
| -109                                                                                | std_tooFewParameters  | Missing parameter - Indicates that less parameters were received than required for the header. For example, *ESE requires one parameter, *ESE is not allowed.                               |
| -110                                                                                | std_cmdHeader         | Command header - Indicates an error was detected in the header. This error is used when the device cannot detect the more specific errors -111 through -119.                                |
| -111                                                                                | std_headerSeparator   | Header separator - Indicates that a character that is not a legal header separator was encountered while parsing the header.                                                                |
| -112                                                                                | std_IDTooLong         | Program mnemonic too long - Indicates that the header contains more that twelve characters, see IEEE 488.2, 7.6.1.4.1.                                                                      |

|      |                         |                                                                                                                                                                                                         |
|------|-------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -113 | std_undefinedHeader     | Undefined header - Indicates the header is syntactically correct, but it is undefined for this specific device. For example, *XYZ is not defined for any device.                                        |
| -114 | std_suffixOutOfRange    | Header suffix out of range - Indicates the value of a header suffix attached to a program mnemonic makes the header invalid.                                                                            |
| -120 | std_numericData         | Numeric data - This error, as well as errors                                                                                                                                                            |
| -121 | std_invalidCharInNumber | Invalid character in number - Indicates an invalid character for the data type being parsed was encountered. For example, an alpha in a decimal numeric or a "9" in octal data.                         |
| -123 | std_exponentTooLarge    | Exponent too large - Indicates the magnitude of an exponent was greater than 32000, see IEEE 488.2, 7.7.2.4.1.                                                                                          |
| -124 | std_decimalTooLong      | Too many digits - Indicates the mantissa of a decimal numeric data element contained more than 255 digits excluding leading zeros, see IEEE 488.2, 7.7.2.4.1.                                           |
| -128 | std_numericNotAllowed   | Numeric data not allowed - Indicates that a legal numeric data element was received, but the device does not accept one in this position for the header.                                                |
| -130 | std_suffix              | Suffix - This error, as well as errors -131 through -139, are generated when parsing a suffix. This particular error message is used if the device cannot detect a more specific error.                 |
| -131 | std_badSuffix           | Invalid suffix - Indicates the suffix does not follow the syntax described in IEEE 488.2, 7.7.3.2, or the suffix is inappropriate for this device.                                                      |
| -134 | std_suffixTooLong       | Suffix too long - Indicates the suffix contain more than 12 characters, see IEEE 488.2, 7.7.3.4.                                                                                                        |
| -138 | std_suffixNotAllowed    | Suffix not allowed - Indicates that a suffix was encountered after a numeric element that does not allow suffixes.                                                                                      |
| -140 | std_charData            | Character data - This error, as well as errors                                                                                                                                                          |
| -141 | std_invalidCharData     | Invalid character data - Indicates that the character data element contains an invalid character or the particular element received is not valid for the header.                                        |
| -144 | std_charDataTooLong     | Character data too long - Indicates the character data element contains more than twelve characters, see IEEE 488.2, 7.7.1.4.                                                                           |
| -148 | std_charNotAllowed      | Character data not allowed - Indicates a legal character data element was encountered where prohibited by the device.                                                                                   |
| -150 | std_stringData          | String data - This error, as well as errors                                                                                                                                                             |
| -151 | std_stringInvalid       | Invalid string data - Indicates that a string data element was expected, but was invalid, see IEEE 488.2, 7.7.5.2. For example, an END message was received before the terminal quote character.        |
| -158 | std_stringNotAllowed    | String data not allowed - Indicates that a string data element was encountered but was not allowed by the device at this point in parsing.                                                              |
| -160 | std_blockData           | Block data - This error, as well as errors -161 through -169, are generated when parsing a block data element. This particular error message is used if the device cannot detect a more specific error. |

|      |                          |                                                                                                                                                                                                               |
|------|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -161 | std_badBlock             | Invalid block data - Indicates a block data element was expected, but was invalid, see IEEE 488.2, 7.7.6.2. For example, an END message was received before the end length was satisfied.                     |
| -168 | std_blockNotAllowed      | Block data not allowed - Indicates a legal block data element was encountered, but not allowed by the device at this point in parsing.                                                                        |
| -170 | std_expr                 | Expression - This error, as well as errors -171 through -179, are generated when parsing an expression data element. This particular error message is used if the device cannot detect a more specific error. |
| -171 | std_invalidExpression    | Invalid expression - Indicates the expression data element was invalid, see IEEE 488.2, 7.7.7.2. For example, unmatched parentheses or an illegal character.                                                  |
| -178 | std_exprNotAllowed       | Expression data not allowed - Indicates a legal expression data was encountered, but was not allowed by the device at this point in parsing.                                                                  |
| -180 | std_macro                | Macro - This error, as well as error -181 through -189, are generated when defining a macro or executing a macro. This particular error message is used if the device cannot detect a more specific error.    |
| -181 | std_validOnlyInsideMacro | Invalid outside macro definition - Indicates that a macro parameter placeholder was encountered outside of a macro definition.                                                                                |
| -183 | std_invalidWithinMacro   | Invalid inside macro definition - Indicates that the program message unit sequence, sent with a *DDT or a *DMC command, is syntactically invalid, see IEEE 488.2, 10.7.6.3.                                   |
| -184 | std_macroParm            | Macro parameter - Indicates that a command inside the macro definition had the wrong number or type of parameters.                                                                                            |

### **-200 to -299 Execution Errors**

These errors are generated when something occurs that is incorrect in the current state of the instrument. These errors may be generated by a user action from either the remote or the manual user interface

|      |                         |                                                                                                                                                                                                                |
|------|-------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -200 | std_execGen             | Execution - This event bit (Bit 4) indicates a PROGRAM DATA element following a header was outside the legal input range or otherwise inconsistent with the device's capabilities, see IEEE 488.2, 11.5.1.1.5. |
| -201 | std_invalidWhileInLocal | Invalid while in local                                                                                                                                                                                         |
| -202 | std_settingsLost        | Settings lost due to rtl                                                                                                                                                                                       |
| -203 | std_commandProtected    | Command protected - Indicates that a legal password-protected program command or query could not be executed because the command was disabled.                                                                 |
| -210 | std_trigger             | Trigger                                                                                                                                                                                                        |
| -211 | std_triggerIgnored      | Trigger ignored                                                                                                                                                                                                |
| -212 | std_armIgnored          | Arm ignored                                                                                                                                                                                                    |
| -213 | std_initIgnored         | Init ignored                                                                                                                                                                                                   |
| -214 | std_triggerDeadlock     | Trigger deadlock                                                                                                                                                                                               |

|      |                        |                                                                                                                                                                                                                                               |
|------|------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -215 | std_armDeadlock        | Arm deadlock                                                                                                                                                                                                                                  |
| -220 | std_parm               | Parameter - Indicates that a program data element related error occurred.                                                                                                                                                                     |
| -221 | std_settingsConflict   | Settings conflict - Indicates that a legal program data element was parsed but could not be executed due to the current device state.                                                                                                         |
| -222 | std_dataOutOfRange     | Data out of range - Indicates that a legal program data element was parsed but could not be executed because the interpreted value was outside the legal range defined by the devices                                                         |
| -223 | std_tooMuchData        | Too much data - Indicates that a legal program data element of block, expression, or string type was received that contained more data than the device could handle due to memory or related device-specific requirements.                    |
| -224 | std_illegalParmValue   | Illegal parameter value - Indicates that the value selected was not part of the list of values given.                                                                                                                                         |
| -225 | std_noMemoryForOp      | Out of memory - The device has insufficient memory to perform the requested operation.                                                                                                                                                        |
| -226 | std_listLength         | Lists not same length - Attempted to use LIST structure having individual LIST's of unequal lengths.                                                                                                                                          |
| -230 | std_dataCorruptOrStale | Data corrupt or stale - Indicates invalid data, a new reading started but not completed since the last access.                                                                                                                                |
| -231 | std_dataQuestionable   | Data questionable - Indicates that measurement accuracy is suspect.                                                                                                                                                                           |
| -232 | std_invalidFormat      | Invalid format                                                                                                                                                                                                                                |
| -233 | std_invalidVersion     | Invalid version - Indicates that a legal program data element was parsed but could not be executed because the version of the data is incorrect to the device. For example, a not supported file version, a not supported instrument version. |
| -240 | std_hardware           | Hardware - Indicates that a legal program command or query could not be executed because of a hardware problem in the device.                                                                                                                 |
| -241 | std_hardwareMissing    | Hardware missing - Indicates that a legal program command or query could not be executed because of missing device hardware. For example, an option was not installed.                                                                        |
| -250 | std_massStorage        | Mass storage - Indicates that a mass storage error occurred. The device cannot detect the more specific errors described for errors -251 through -259.                                                                                        |
| -251 | std_missingMassStorage | Missing mass storage - Indicates that a legal program command or query could not be executed because of missing mass storage.                                                                                                                 |
| -252 | std_missingMedia       | Missing media - Indicates that a legal program command or query could not be executed because of missing media. For example, no disk.                                                                                                         |
| -253 | std_corruptMedia       | Corrupt media - Indicates that a legal program command or query could not be executed because of corrupt media. For example, bad disk or wrong format.                                                                                        |



|      |                            |                                                                                                                                                                                                                       |
|------|----------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -254 | std_mediaFull              | Media full- Indicates that a legal program command or query could not be executed because the media is full. For example, there is no room left on the disk.                                                          |
| -255 | std_directoryFull          | Directory full - Indicates that a legal program command or query could not be executed because the media directory was full.                                                                                          |
| -256 | std_fileNotFound           | File name not found - Indicates that a legal program command or query could not be executed because the file name was not found on the media.                                                                         |
| -257 | std_fileName               | File name - Indicates that a legal program command or query could not be executed because the file name on the device media was in error. For example, an attempt was made to read or copy a nonexistent file.        |
| -258 | std_mediaProtected         | Media protected - Indicates that a legal program command or query could not be executed because the media was protected. For example, the write-protect switch on a memory card was set.                              |
| -260 | std_expression             | Expression                                                                                                                                                                                                            |
| -261 | std_math                   | Math in expression                                                                                                                                                                                                    |
| -270 | std_macroExecution         | Macro - Indicates that a macro related execution error occurred.                                                                                                                                                      |
| -271 | std_macroSyntax            | Macro syntax - Indicates that a syntactically legal macro program data sequence, according to IEEE 488.2, 10.7.2, could not be executed due to a syntax error within the macro definition.                            |
| -272 | std_macroExec              | Macro execution - Indicates that a syntactically legal macro program data sequence could not be executed due to some error in the macro definition, see IEEE 488.2, 10.7.6.3.                                         |
| -273 | std_badMacroName           | Illegal macro label - Indicates that the macro label was not accepted, it did not agree with the definition in IEEE 488.2, 10.7.3                                                                                     |
| -274 | std_macroPlaceholder<br>Ma | cro parameter - Indicates that the macro definition improperly used a macro parameter placeholder, see IEEE 488.2, 10.7.3.                                                                                            |
| -275 | std_macroTooLong           | Macro definition too long - Indicates that a syntactically legal macro program data sequence could not be executed because the string of block contents were too long for the device to handle, IEEE 488.2, 10.7.6.1. |
| -276 | std_macroRecursion         | Macro recursion - Indicates that a syntactically legal macro program data sequence count not be executed because it would be recursive, see IEEE 488.2, 10.7.6.6.                                                     |
| -277 | std_cantRedefineMacro      | Macro redefinition not allowed - Indicates that redefining an existing macro label, see IEEE 488.2, 10.7.6.4.                                                                                                         |
| -278 | std_macroNotFound          | Macro header not found - Indicates that a legal macro label in the *GMS?, see IEEE 488.2, 10.13, could not be executed because the header was not previously defined.                                                 |
| -280 | std_program                | Program                                                                                                                                                                                                               |

|      |                        |                                |
|------|------------------------|--------------------------------|
| -281 | std_cantCreateProgram  | Cannot create program          |
| -282 | std_illegalProgramName | Illegal program name           |
| -283 | std_illegalVarName     | Illegal variable name          |
| -284 | std_programRunning     | Program currently running      |
| -285 | std_programSyntax      | Program syntax                 |
| -286 | std_programRuntime     | Program runtime                |
| -290 | std_memoryUse          | Memory use                     |
| -291 | std_execOutOfMemory    | Out of memory                  |
| -292 | std_nameNotFound       | Referenced name does not exist |
| -293 | std_nameAlreadyExists  | Referenced name already exists |
| -294 | std_incompatibleType   | Incompatible type              |

### **-300 to -399 SCPI Specified Device-Specific Errors**

A device-specific error indicates that the instrument has detected an error that occurred because some operations did not properly complete, possibly due to an abnormal hardware or firmware condition. For example, an attempt by the user to set an out of range value will generate a device specific error. When one of these errors is generated, the device specific error bit in the event status register is set.

|      |                      |                                                                                                                                                                            |
|------|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -300 | std_deviceSpecific   | Device specific - This event bit (Bit 3) indicates that a device operation did not properly complete due to some condition, such as overrange see IEEE 488.2, 11.5.1.1.6.  |
| -310 | std_system           | System                                                                                                                                                                     |
| -311 | std_memory           | Memory - Indicates some physical fault in the devices memory, such as a parity error.                                                                                      |
| -312 | std_PUDmemoryLost    | PUD memory lost - Indicates protected user data saved by the *PUD command has been lost, see IEEE 488.2, 10.27.                                                            |
| -313 | std_calMemoryLost    | Calibration memory lost - Indicates that nonvolatile calibration data used by the *CAL? command has been lost, see IEEE 488.2, 10.2.                                       |
| -314 | std_savRclMemoryLost | Save/recall memory lost - Indicates that the nonvolatile data saved by the *SAV command has been lost, see IEEE 488.2, 10.33.                                              |
| -315 | std_configMemoryLost | Configuration memory lost - Indicates that nonvolatile configuration data saved by the device has been lost.                                                               |
| -320 | std_storageFault     | Storage fault - Indicates that the firmware detected a fault when using data storage. This is not an indication of physical damage or failure of any mass storage element. |
| -321 | std_outOfMemory      | Out of memory - An internal operation needed more memory than was available                                                                                                |

|                             |                                                                                                                                                                                          |
|-----------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -330 std_selfTestFailed     | Self-test failed - Indicates a problem with the device that is not covered by a specific error message. The device may require service.                                                  |
| -340 std_calFailed          | Calibration failed - Indicates a problem during calibration of the device that is not covered by a specific error.                                                                       |
| -350 std_queueOverflow      | Queue overflow - Indicates that there is no room in the queue and an error occurred but was not recorded. This code is entered into the queue in lieu of the code that caused the error. |
| -360 std_comm               | Communication - This is the generic communication error for devices that cannot detect the more specific errors described for error -361 through -363.                                   |
| -361 std_parity             | Parity in program message - Parity bit not correct when data received for example, on a serial port.                                                                                     |
| -362 std_framing            | Framing in program message - A stop bit was not detected when data was received for example, on a serial port (for example, a baud rate mismatch).                                       |
| -363 std_inputBufferOverrun | Input buffer overrun - Software or hardware input buffer on serial port overflows with data caused by improper or nonexistent pacing.                                                    |

#### **-400 to -800 Query and System Errors**

A Query error is generated either when data in the instrument's GPIB output queue has been lost, or when an attempt is being made to read data from the output queue when no output is present or pending.

|                             |                                                                                                                                                                                                         |
|-----------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| -400 std_queryGen           | Query - This event bit (Bit 2) indicates that an attempt to read data from the Output Queues when no output is present or pending, to data in the Output Queue has been lost see IEEE488.2, 11.5.1.1.7. |
| -410 std_interrupted        | Query INTERRUPTED - Indicates the test set has been interrupted by a new program message before it finishes sending a RESPONSE MESSAGE see IEEE 488.2, 6.3.2.3.                                         |
| -420 std_unterminated       | Query UNTERMINATED - Indicates an incomplete Query in the program see IEEE 488.2, 6.3.2.2.                                                                                                              |
| -430 std_deadlocked         | Query DEADLOCKED - Indicates that the Input Buffer and Output Queue are full see IEEE 488.2, 6.3.1.7.                                                                                                   |
| -440 std_responseNotAllowed | Query UNTERMINATED after indefinite response - Indicates that a query was received in the same program message after a query requesting an indefinite response was executed see IEEE 488.2, 6.5.7.5.    |
| -500 std_powerOn            | Power on                                                                                                                                                                                                |
| -600 std_userRequest        | User request                                                                                                                                                                                            |
| -700 std_requestControl     | Request control                                                                                                                                                                                         |
| -800 std_operationComplete  | Operation complete                                                                                                                                                                                      |

#### **PNA Specific SCPI Errors**

|                             |                                                                        |
|-----------------------------|------------------------------------------------------------------------|
| 100 dupWindNum              | "Duplicate window number"                                              |
| 101 windNumNotFound         | "Window number not found"                                              |
| 102 failedWindCreate        | "Window creation failed"                                               |
| 103 noCalcParamSelection    | "CALC measurement selection set to none"                               |
| 104 dupMeasName             | "Duplicate measurement name"                                           |
| 105 dataNotFound            | "Requested data not available"                                         |
| 106 measNotFound            | "Requested measurement not found"                                      |
| 107 traceNotFound           | "Requested trace not found"                                            |
| 108 notImplemented          | "Mnemonic not yet implemented"                                         |
| 109 noDocument              | "No measurement container found"                                       |
| 110 dupTraceNum             | "Duplicate trace number"                                               |
| 111 titleStrTooLong         | "Title string exceeds 50 characters"                                   |
| 112 memoryNotFound          | "Requested memory not found"                                           |
| 113 exceedMaxTraces         | "Exceeded the maximum number of traces per window"                     |
| 114 SerNumNotFound          | "The serial number was not found. Please store the serial number."     |
| 115 LoadFailed              | "The state was not loaded. Please check the file name."                |
| 116 StoreFailed             | "The state was not stored. Please check the file and path names."      |
| 117 File                    | "An in the File operation occurred. Please check file and path names." |
| 118 measChanConflict        | "Measurement does not belong to specified channel."                    |
| 119 exceedMaxWindows        | "Exceeded the maximum number of data windows"                          |
| 120 markerNotFound          | "The specified marker was not found."                                  |
| 121 diagnostic              | "Diagnostic ."                                                         |
| 122 channelNotFound         | "The specified channel was not found."                                 |
| 123 exceedMaxMeasurements   | "Exceeded the maximum number of allowed measurements."                 |
| 124 parameterOutOfRange     | "The specified value was out of range."                                |
| 125 userRangeNotValid       | "The currently selected user range is not valid."                      |
| 126 referenceMarkerNotFound | "The reference marker is not active."                                  |
| 127 sweepSegmentNotFound    | "The sweep segment was not found."                                     |

|     |                             |                                                         |
|-----|-----------------------------|---------------------------------------------------------|
| 128 | markerNotDelta              | "The specified marker is not a delta marker."           |
| 129 | printoutFailed              | "Attempt to output to a printer failed."                |
| 130 | memory_trace_not_compatible | "Memory not compatible. Trace Math not applied."        |
| 131 | trace_math_reset            | "Memory not compatible. Trace Math turned off."         |
| 132 | hw_read_failed              | "Hardware read failed."                                 |
| 133 | hw_write_failed             | "Hardware write failed."                                |
| 134 | dsp_active                  | "Failed because DSP was not halted."                    |
| 135 | secure_memory               | "Attempt to access secure memory region."               |
| 136 | snum_protected              | "The serial number is protected."                       |
| 137 | snum_format_bad             | "The serial number format is bad."                      |
| 138 | snum_already_set            | "The serial number is already set."                     |
| 139 | hw_setting_failed           | "Hardware setting failed."                              |
| 140 | cal_access_failed           | "Calibration data access failed."                       |
| 141 | db_access_failed            | "Database access failed."                               |
| 142 | memory_range_exceeded       | "Command exceeds usable memory range."                  |
| 143 | lost_phase_lock             | "Phase lock has been lost."                             |
| 144 | over_power                  | "Detected too much power at input."                     |
| 145 | ee_wrt_failed               | "EEPROM write failed."                                  |
| 146 | yig_cal_failed              | "YTO calibration failed."                               |
| 147 | ramp_cal_failed             | "Analog ramp calibration failed."                       |
| 148 | dspcom_bad                  | "DSP communication failed."                             |
| 149 | no_license_found            | "Request failed. The required license was not found."   |
| 150 | argLimited                  | "The argument was out of range"                         |
| 151 | markerBWNotFound            | "The Marker Bandwidth was not found."                   |
| 153 | peakNotFound                | "The Peak was not found."                               |
| 154 | targetNotFound              | "The Target search value was not found."                |
| 155 | calNotImpl                  | "The Calibration feature requested is not implemented." |
| 156 | calClassNotValidForCalType  | "SENS:CORR:CCH measurement selection set to none"       |

|     |                                  |                                                                                                                           |
|-----|----------------------------------|---------------------------------------------------------------------------------------------------------------------------|
| 158 | calNotValidForConfidenceChe      | "Selected measurement does not have a calibration valid for Confidence Check"                                             |
| 159 | invalidPort                      | "Specified port is out of range"                                                                                          |
| 160 | invalidPortPath                  | "ROUT:PATH:DEF:PORT x, y does not match measurement; setting to defaults"                                                 |
| 161 | ioInvalidWrite                   | "Attempted I/O write while port set to read only."                                                                        |
| 162 | ioInvalidRead                    | "Attempted I/O read from write only port."                                                                                |
| 163 | calsetNotFound                   | "Requested Cal Set was not found in Cal Set Storage."                                                                     |
| 164 | noCalSetSelected                 | "There is no Cal Set currently selected for the specified channel."                                                       |
| 165 | cantDeleteCalSetInUse            | "Cannot delete a Cal Set while it is being used."                                                                         |
| 166 | calsetStimChange                 | "Channel stimulus settings changed to match selected Cal Set."                                                            |
| 167 | exceedMaxCalSets                 | "Exceeded the maximum number of cal sets."                                                                                |
| 168 | calCouldNotTurnOn                | "A valid calibration is required before correction can be turned on."                                                     |
| 169 | standardMeasurementRequired      | "The attempted operation can only be performed on a standard measurement type."                                           |
| 170 | noDivisorBuffer                  | "A valid divisor buffer is required before normalization can be turned on."                                               |
| 171 | InvalidReceiverPowerCalParagraph | "Receiver power cal requires the measurement to be of unratiod power."                                                    |
| 172 | ecalCouldNotConfigure            | "Could not configure the Electronic Calibration system. Check to see if the module is plugged into the proper connector." |
| 173 | measHasNoMemoryAlg               | "This measurement does not support memory operations"                                                                     |
| 174 | measHasNoNormalizeAlg            | "This measurement does not support normalize operations."                                                                 |
| 175 | userCharacterizationNotFound     | "User characterization was not found in the Electronic Calibration module."                                               |
| 176 | measInvalidBufferSize            | "The data provided has an invalid number of points. It could not be stored."                                              |

## Technical Support

---

Click on the region of interest.



- For assistance with your test and measurement needs go to [www.agilent.com/find/assist](http://www.agilent.com/find/assist)
- Or contact the test and measurement experts at Agilent Technologies.

### Other Support Topics

#### United States:

(tel) (+1) 800 452 4844  
(alt) (+1) 303 662 3999  
(fax) (+1) 888 900 8921

#### Canada

(tel) 1 877 894 4414  
(fax) 1 (905) 206 4120

#### rope:

##### Austria

(tel) 0820 87 44 11\*  
(fax) 0820 87 44 22

##### Belgium

(tel) (+32) (0)2 404 9340  
(alt) (+32) (0)2 404 9000  
(fax) (+32) (0)2 404 9395

##### Denmark

(tel) (+45) 7013 1515  
(alt) (+45) 7013 7313  
(fax) (+45) 7013 1555

**Finland**

(tel) 08 0052 4000

(alt) (+358) 10 855 2100

(fax) (+358) 92 536 0176

**France**

(tel) 0825 010 700\*

(alt) (+33) (0)1 6453 5623

(fax) 0825 010 701\*

**Germany**

(tel) 01805 24 6333\*

(alt) 01805 24 6330\*

(fax) 01805 24 6336\*

**Ireland**

(tel) (+353) (0)1 890 924 204

(alt) (+353) (0)1 890 924 206

(fax) (+353) (0)1 890 924 024

**Israel**

(tel) (+972) 3 9288 500

(fax) (+972) 3 9288 501

**Italy**

(tel) (+39) (0)2 9260 8484

(fax) (+39) (0)2 9544 1175

**Luxemburg**

(tel) (+32) (0)2 404 9340

(alt) (+32) (0)2 404 9000

(fax) (+32) (0)2 404 9395

**Netherlands**

(tel) (+31) (0)20 547 2111

(alt) (+31) (0)20 547 2000

(fax) (+31) (0)20 547 2190

**Russia**

(tel) (+7) 095 797 3963

(alt) (+7) 095 797 3900

(fax) (+7) 095 797 3901



**Spain**

(tel) (+34) 91 631 3300

(alt) (+34) 91 631 3000

(fax) (+34) 91 631 3301

**Sweden**

(tel) 0200 88 22 55\*

(alt) (+46) (0)8 5064 8686

(fax) 020 120 2266\*

**Switzerland (French)**

(tel) 0800 80 5353 opt. 2\*

(alt) (+33) (0)1 6453 5623

(fax) (+41) (0)22 567 5313

**Switzerland (German)**

(tel) 0800 80 5353 opt. 1\*

(alt) (+49) (0)7031 464 6333

(fax) (+41) (0)1 272 7373

**Switzerland (Italian)**

(tel) 0800 80 5353 opt. 3\*

(alt) (+39) (0)2 9260 8484

(fax) (+41) (0)22 567 5314

**United Kingdom**

(tel) (+44) (0)7004 666666

(alt) (+44) (0)7004 123123

(fax) (+44) (0)7004 444555

**Japan:**

(tel) 0120 421 345

(alt) (+81) 426 56 7832

(fax) 0120 421 678

**Latin America:****Mexico**

(tel) (+52) 55 5081 9469

(alt) 01800 5064 800

(fax) (+52) 55 5081 9467

**Brazil**

(tel) (+55) 11 4197 3600

(fax) (+55) 11 4197 3800

### **Australia:**

((tel) 1800 629 485

(alt) 1800 143 243

(fax) 1800 142 134

### **New Zealand**

(tel) 0 800 738 378

(fax) 64 4 495 8950

### **Asia Pacific:**

#### **China**

(tel) 800 810 0189

(alt) (+86) 10800 650 0021

(fax) 800 820 2816

#### **Hong Kong**

(tel) 800 930 871

(alt) (+852) 3197 7889

(fax) (+852) 2 506 9233

#### **India**

(tel) 1600 112 929

(fax) 000800 650 1101

#### **Malaysia**

(tel) 1800 888 848

(alt) 1800 828 848

(fax) 1800 801 664

#### **Singapore**

(tel) 1800 375 8100

(fax) (+65) 6836 0252

#### **South Korea**

(tel) 080 769 0800

(alt) (+82) 2 2004 5004

(fax) (+82) 2 2004 5115

#### **Taiwan**

(tel) 0800 047 866

(alt) 00801 651 317

(fax) 0800 286 331

**Thailand**

(tel) 1800 226 008

(alt) (+66) 2 268 1345

(fax) (+66) 2 661 3714

## 3.8 GHz Frequency Adjustment

---

This routine adjusts the internal fixed-frequency YIG Oscillator to 3.8 GHz by changing a DAC value. This DAC value is stored in the analyzer's non-volatile memory.

Typically, the oscillator can be set to within 12 kHz of 3.8GHz; it is not necessary for it to be exactly 3.8GHz.

### Spectrum Analyzers Compatibility

This routine is compatible with Agilent 856x and 859x spectrum analyzers.

If no compatible analyzer is available, select "NONE" for the spectrum analyzer. You can then adjust the DAC manually by viewing the 3.8 GHz signal on another analyzer.


### Procedure (For Compatible Spectrum Analyzers Only)

---

**Note:** The viewable 3.8 GHz signal level will be low; typically be around -70dBm. Do not use any attenuators in the adjustment, other than the default 10 dB attenuation used in most spectrum analyzers.

---

1. Connect spectrum analyzer input to the network analyzer's PORT 1 output.
2. Connect GPIB cable from analyzer to spectrum analyzer. Make sure no other controllers are active on the same connection.

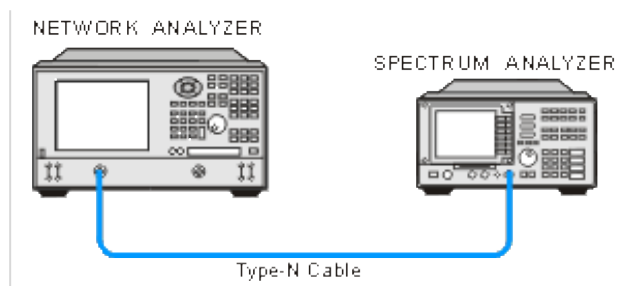

3. Set the spectrum analyzer GPIB address to 18.
4. In the analyzer **System** menu, point to **Service, Adjustments**, and click **3.8 GHz Freq. Adjust**.
5. Click **Begin Adj.** for the program to adjust the internal oscillator for minimal error and store the results. When the status area indicates the adjustment is complete, select **Exit**.

### Procedure (For Non-Compatible Spectrum Analyzers Only)

---

**Note:** The viewable 3.8 GHz signal level will be low; typically be around -70dBm. Do not use any attenuators in the adjustment, other than the default 10 dB attenuation used in most spectrum analyzers.

---

1. Connect the spectrum analyzer input to the network analyzer's PORT 1 output.
2. Set the spectrum analyzer to the following settings:
  - Center frequency=3.8 GHz
  - Span= 100 MHz
  - Bandwidth= 10 kHz

- Scaling where a signal of -70 dBm will be clearly visible
3. In the analyzer **System** menu, point to **Service, Adjustments**, and click **3.8 GHz Freq. Adjust**.
  4. Under **Spectrum Analyzer**, select **NONE** option for spectrum analyzer.
  5. Click **Begin Adj.**
  6. The application presets the DAC to an initial value equal to the current value stored. View the spectrum analyzer to see if the signal is above or below 3.800 GHz.
    - If the signal frequency is above 3.8 GHz, move the slider to adjust the DAC to a lower value (left).
    - If the frequency is below 3.8 GHz, move the slider to adjust the DAC to a higher value (right).

---

**Note:** The valid DAC values are from 0 to 4095. The oscillator will shift about 23 kHz per DAC value.

---

7. Set the DAC value to reach a frequency very close to 3.8 GHz. If you made large changes in DAC values, allow several seconds for thermal effects to stabilize.
8. Change the spectrum analyzer settings to better view the frequency signal:
  - Frequency span = 500 kHz
  - Bandwidth = 3 kHz
9. Change the DAC value to keep the signal centered at 3.8 GHz.
10. Once you have determined the correct DAC value, click **SAVE DAC** to permanently store that value into EEPROM. Click **Exit**.

---

**Note:** If large changes are made to the existing DAC value, then this test should be repeated again after 15-30 minutes. This allows the thermal effects to fully stabilize.

---

## 10 MHz Reference Frequency Adjustment

---

This routine adjusts the analyzer's internal time-base to exactly 10 MHz by changing a DAC value. This DAC value is stored in the analyzer's non-volatile memory. This routine should only be necessary in the following situations:

- The frequency reference assembly is replaced.
- The 10 MHz reference has drifted significantly from the factory adjusted value.

**WARNING:** The range of this adjustment is only about 20 Hz. It is highly recommended that a very accurate frequency standard be used to measure this 10 MHz signal.

### Frequency Counter Compatibility

This procedure uses SCPI commands (over GPIB) to communicate with the frequency counter. It should work with the Agilent 5313xA, 5315xA, 53181A series of counters as well as the older 5350 series.

If no compatible counters are available, select the "Manual" mode of operation. If you do choose the manual mode, you must input the measured frequency manually.

### Procedure for GPIB Counters Only

1. Connect the analyzer rear panel 10 MHz Reference output to the frequency counter .
2. Connect a GPIB cable from the analyzer to the counter. Make sure no other controllers are active on the same connection.
3. If applicable, connect the house frequency standard to the counter reference input.
4. Set the counter GPIB address to 03. Ensure that the counter is the only device at this address.
5. In the analyzer **System** menu, point to **Service, Adjustments**, and click **10 MHz Freq. Adjust**.
6. Click **Begin Adj**. The application adjusts the internal reference for minimal error and stores the results.
7. Click **Read Freq** to trigger another reading of the 10 MHz signal.
8. Click **Read DAC** to view the current DAC value stored in the analyzer's non-volatile memory (value = 0 - 4095).
9. When the status area indicates the adjustment is complete, click **Exit**.

### Procedure for Non-GPIB Counters

1. Connect the counter input to the rear panel 10 MHz Reference Output.
2. Set the counter to at least 1 Hz resolution.
3. If applicable, connect the house-frequency standard to the counter reference input.
4. In the analyzer **System** menu, point to **Service, Adjustments** and click **10 MHz Freq. Adjust**.
5. Under **Frequency Counter**, select **Manual**.
6. Click **Begin Adj**.

7. The application presets the DAC to an initial value. Enter the measured frequency offset from 10 MHz. If the measured frequency is less than 10 MHz, use a minus (-) sign to indicate a negative error. For example:
  - If the counter reads 10000003.5 Hz, enter 3.5 (or +3.5) in the indicated window.
  - If the counter reads 9999997.8 Hz, enter -2.2 in the indicated window.
8. The adjustment loops at least 3 times unless the entered value is exactly zero.
  - Click **Read Freq** to trigger another reading of the 10 MHz signal.
  - Click **Read DAC** to view the current DAC value stored in the analyzer's non-volatile memory (value = 0 - 4095).
9. When the status area indicates the adjustment is complete, click **Exit**.

---

**Note:** If the counter is misreading the frequency, it may be necessary to attenuate the input, or set the input impedance to 50 ohms, or both.

---

## LO Power Adjustment

---

This procedure adjusts the receiver's LO input power to a specific level by changing DAC values. These DAC values are then stored in the analyzer's non-volatile memory. The procedure will vary depending upon the model number.

### Power Meter Compatibility

This routine is only compatible with the Agilent EPM series of power meters. Different sensors may be used. For 9 GHz analyzers and below, an 8482 or E4412A sensor can be used. For the higher frequency units (20 GHz or above), a sensor must be able to measure a maximum of 20 GHz. At no time during this test will a frequency higher than 20 GHz be measured, even if the PNA has a maximum frequency of 50 GHz.

If the older HP 84xx series of sensors are used, the correct calibration data should be entered into the appropriate cal table of the EPM series power meter, although for this adjustment, high accuracy is not required. Inaccuracies in the order of several tenths of a dB are acceptable.

### Procedure

1. Allow the analyzer and power meter to warm up for 30 minutes.
2. Manually zero and calibrate the power sensor. (This allows you to skip this step later)
3. Connect a GPIB cable from the analyzer to the power meter. Make sure no other controllers are active on the same connection.
4. Set the power meter GPIB address to 13. (others can also be used; 13 is the default)
5. Remove the outer cover on the analyzer.
6. In the PNA **System** menu point to **Service**, then **Adjustments**, and click **LO Power Adjust**.
7. Connect the power sensor to the LO output, using adapters if needed.. The LO output location varies with model number. Click on the LO Power Adjust **Setup** menu selection to see a diagram of the exact location.
8. **For 9 GHz units and below:**  
Click **Begin Adj** to start the LO power cal routine. The routine adjusts the power level for each band (1 through 3) to fall within certain bounds. If any changes are made, it automatically stores them.  
  
**For 20GHz units and above:**  
If using an 84xx power sensor, click **Configure** and select the proper sensor model number. Click **Close**. Click **Calibrate** to begin the adjustment. The entire calibration process takes about 5 minutes. Once completed, you can verify the current calibration accuracy by clicking **Verify Cal**.  
**Note:** Correction constants are defaulted at the beginning of calibration. Once the calibration process has started, it must be completed in order to regenerate proper data.
9. Click **Read DAC** to view the current DAC values (0-4095) stored in the PNA non-volatile memory for each band (0-7).
10. When the message/status area indicates the adjustment is complete, click **Exit**.
11. Reconnect the semi-rigid cable and replace the covers.





## Offset LO Power Adjustment

---

**Note:** This adjustment is only performed on PNAs with Frequency Offset Mode (option 080).

The Offset LO Adjustment sets the LO power for the offset mixer to a consistent value across all bands. It requires access to the internal components of the PNA so that the power sensor can be connected to the LO output.

Because the LO frequency does not exceed 3 GHz, almost any power sensor can be used. The adjustment is relatively simple and only takes a couple of minutes.

### When to perform

This adjustment should be performed when any of the following occur:

- the A13 Frequency Offset Receiver is significantly modified or replaced
- the A9 Synthesizer is replaced (that is where the correction data resides)

### How to perform Offset LO Power adjustment

1. To start the Offset LO adjustment, click **System**, point to **Service, Adjustments**, then click **Offset LO Adjust**.
2. You will be prompted to zero and cal the power sensor. (You can do this before beginning.)
3. Connect the sensor to J3 of the A13 LO output by removing the existing cable (or simply disconnecting one end) as shown in the Set-up diagram in the program.
4. Connect the power meter to the PNA using a GPIB cable. Make sure the GPIB address shown in the program matches the actual power meter address (default is 13.)
5. Click **Adjust** to begin the test and follow the instructions.

The program automatically adjusts all bands; no user input is needed. The program repeats several times as this is an iterative process. The progress of the adjustment is shown on the screen.

The Configure menu selection is for factory personnel ONLY.

Once completed, to verify the actual results, click Verify.

Upon exiting, the PNA application will restart; this takes several seconds.

# Operator's Check

---

## [Overview](#)

## [How to Run the Operator's Check](#)

## [Operators Check Dialog Box Help](#)

### Overview

The Operator's Check should be performed when you first receive your PNA, and any time you wish to have confidence that the PNA is working properly.

---


**Note:** The Operator's Check does not verify performance to specifications. To verify PNA performance to specifications, run [System Verification](#).

---

The Pass/Fail criteria used in the Operator's Check identifies **obvious failures** in the following portions of the PNA hardware:


- Repeatability of the RF switch in the test set
- Attenuation ranges of the test port attenuators (if installed)
- Calibration of the receivers
- Frequency response of the receivers
- Phase lock and leveling
- Noise floor and trace noise

### How to Run the Operator's Check

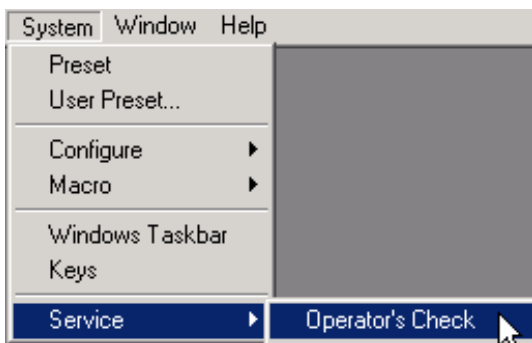

1. Click **Service** and **Operator's Check**.
2. Connect one or more standards (see [Configure](#)).
3. Click **Begin** and **Continue** (if necessary) until "Operator's Check is complete!" appears.

Learn more about using the [front panel interface](#)

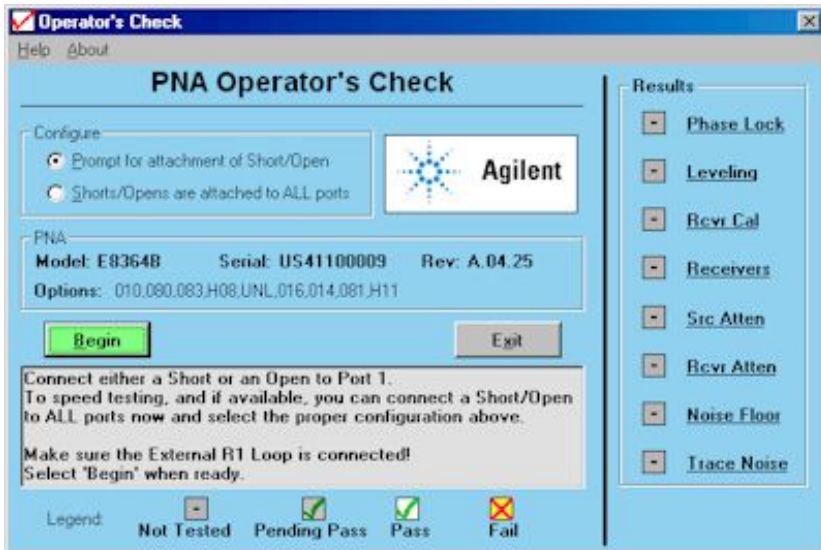

This dialog box will look slightly different, depending on PNA model number and installed options. Some of the tests are not run if the appropriate option is not installed.

## Operators Check dialog box help

### Configure

**Prompt for attachment of Short / Open** If you do not have enough shorts or opens for all test ports, you will be prompted to move the standard to the next test port. Connect either a short or open to port 1, then click Begin.

**Shorts / Opens are attached to all ports** Connect either a short or open for each test port, then click Begin. All ports are tested without interruption. You can mix shorts and opens on the test ports.

**PNA** Shows information about the PNA that is being tested.

**Legend** Shows the status icons used in the Operator's Check and their meaning. **Pending Pass** means that a portion of the testing has been completed successfully.

**Results** Shows the current status of each test. Click on the test name to learn how that test is performed. This may help in troubleshooting failed tests. If any tests Fail, refer to Chapter 3 of the PNA service guide.

**Begin** Starts the Operator's Check.

**View Results** Shows all results in text format. Failed items are preceded by ==>>>>.

This text file can be printed or saved with a unique file name to compare results with previous or subsequent testing.

**Exit** Ends the program and closes the window.


## Option H11 Verification

The PNA Option H11 verification utility verifies the H11 operation by measuring the associated inputs and outputs and comparing the results against Factory standards. These tests can be used in conjunction with the [Operator's Check](#).


- [How to Run Option H11 Verification](#)
- [Option H11 Verification Dialog Help](#)

### [Test Set Tester](#)

### How to Run Option H11 Verification

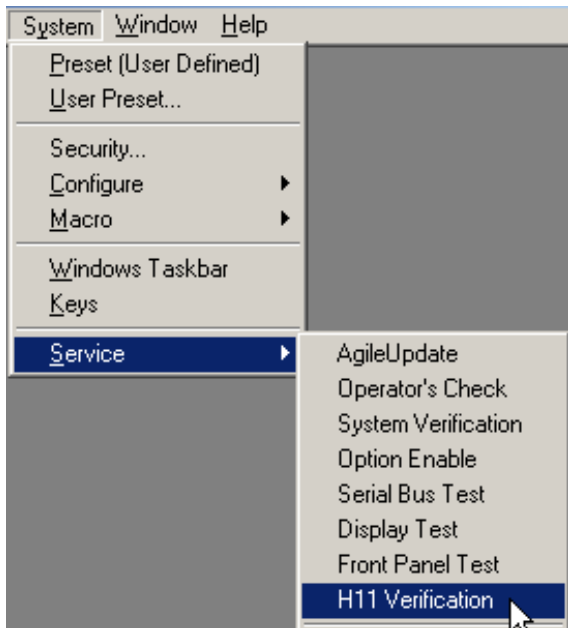

Learn more about using the [front panel interface](#)

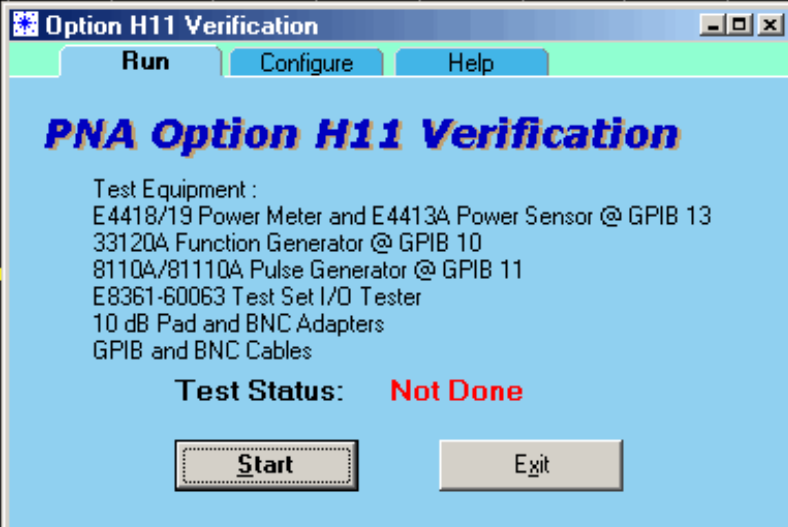

**Option H11 Verification**

Run    Configure    Help

**PNA Option H11 Verification**

Test Equipment :  
E4418/19 Power Meter and E4413A Power Sensor @ GPIB 13  
33120A Function Generator @ GPIB 10  
81110A/81111QA Pulse Generator @ GPIB 11  
E8361-60063 Test Set I/O Tester  
10 dB Pad and BNC Adapters  
GPIB and BNC Cables

**Test Status: Not Done**

Start    Exit

### Run Tab

The test equipment is the complete list that is required to run ALL of the tests.

**Start** Click to begin the tests that are checked on the Configure Tab

**Exit** Exits the Utility

### Configure Tab

Check to select the tests you would like to run.

**Power Tests** Checks power at the selected connectors on the rear panel. The results displayed against limit lines that represent the expected levels at the factory.

Equipment Required:

- PNA supported power meter and power sensor
- GPIB and Sensor cables
- E8361A only: Testset I/O tester

**External IF Input and Crosstalk Tests** A 8.33 MHz signal is injected into the External IF input. The signal is measured at each of the selected receivers. The results displayed against limit lines that represent the expected levels at the factory.

Equipment Required:

- 33120A function Generator
- 10 dB attenuator (Agilent 8493B or equivalent) and BNC adapters
- GPIB and BNC cables

**External Pulse Input Test** A pulse train is injected into the Pulse input connector. The signal is measured at each of the selected receivers. The results displayed against limit lines that represent the expected levels at the factory.

Equipment Required:

- 8110A81110A Pulse Generator
- GPIB and BNC cables

**Test Set I/O Connector Test** Does this and that to the connector.

Equipment Required:

- Testset I/O tester

**Test Set I/O tester**

A description of what this thing is and how to put it together.

## Phase-Lock IF Gain Adjustment

---

The E836x A/B PNA models have a variable gain control for the phase-lock loop IF signal. By dynamically changing the gain as a function of frequency and power, the phase-lock signal amplitude can be adjusted to a constant level for the entire operating range of the instrument. This constant level is important for phase-lock acquisition and stability.

### When to perform

Phase-Lock IF Gain Adjustment should be performed when any of the following occur:

- a source calibration
- an assembly in the reference receiver path (R1,R2) is replaced.
- the Test Set Motherboard is replaced
- the Phase Lock board is replaced
- **Phase Lock Lost** error message appears after replacing a source or receiver assembly

### How to perform Phase-Lock IF Gain adjustment

1. From the **System** menu, click **Service**, then **Adjustments**, then **IF Gain Adjustment**.
2. Select any special test set options installed, otherwise leave the selection at **None**.
3. No connections to the test ports are required.
4. Click **Begin Adj**. The adjustment takes about a minute to complete.
5. The advanced screen is for factory personnel only.



## System Verification

---

The system verification utility verifies the PNA system specifications by automatically measuring the magnitude and phase for all four S-parameters for each verification device, and comparing the values against the following:

- Factory measured data from files on the verification disk
- Limit lines based on the measurement uncertainty

System Verification requires the use of a calibration kit and verification kit which have been recently certified using a NIST-traceable process. System Verification can NOT be used to perform this kit certification.

Operator's Check should also be performed to verify the basic operation of the PNA.

### Equipment Used in the System Verification

### Precautions for Handling Airlines

### Flow Diagram of Procedure

### Procedure for System Verification

### If the System Fails the Verification Test

### Interpreting the Verification Results

---

**Note:** Although the performance for all S-parameters is measured, the S<sub>11</sub>, S<sub>22</sub>, S<sub>33</sub>, and S<sub>44</sub> phase uncertainties are less important for verifying system performance. Therefore, the limit lines will not appear on the printouts.

---

## Equipment Used in the System Verification

For PNA models:

**E8356A, E8357A, E8358A**

**N3381A, N3382A, N3383A**

**E8801A, E8802A, E8803A**

(Type-N test ports)

| Equipment Type                       | Type-N               | 3.5 mm                        |
|--------------------------------------|----------------------|-------------------------------|
| Calibration kit<br>or<br>ECAL Module | 85032F<br><br>85092B | 85033E<br><br>85093B          |
| Verification kit                     | 85055A               | 85053B                        |
| RF Cable                             | N6314A               | <u>See Cable substitution</u> |

**E8362A/B**

**N5230A (20 GHz)**

(3.5 mm test ports)

| Equipment Type                       | 3.5 mm                             | Type-N                                                                                                                   |
|--------------------------------------|------------------------------------|--------------------------------------------------------------------------------------------------------------------------|
| Calibration kit<br>or<br>ECAL Module | 85052B/C/D<br>N4691A               | 85054B/D<br>N4690A                                                                                                       |
| Verification kit                     | 85053B                             | 85055A                                                                                                                   |
| RF Cable(s)                          | Single: 85131C/E<br>Pair: 85131D/F | Single: 85132C/E<br>Pair: 85132D/F                                                                                       |
| Adapters                             | None                               | Single: 85130C and one<br>7mm-to-Type-N from<br>85054B cal kit<br><u>Pair:</u> Two 7mm-to-Type-<br>N from 85054B cal kit |

**E8363A/B, E8364A/B**  
**N5230A (40 or 50 GHz)**  
(2.4 mm test ports)

| Equipment Type                       | 2.4 mm                             | 3.5 mm                                     | Type-N                                                                                                                             |
|--------------------------------------|------------------------------------|--------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------|
| Calibration kit<br>or<br>ECAL Module | 85056A/D<br>N4693A                 | 85052B/C/D<br>N4691A                       | 85054B/D<br>N4690A                                                                                                                 |
| Verification kit                     | 85057B                             | 85053B                                     | 85055A                                                                                                                             |
| RF Cable(s)                          | Single: 85133C/E<br>Pair: 85133D/F | Single: 85134C/E<br>Pair: 85134D/F         | Single: 85135C/E<br>Pair: 85135D/F                                                                                                 |
| Adapters                             | None                               | <u>Single:</u> 85130F<br><u>Pair:</u> None | <u>Single:</u> 85130E and<br>two 7mm-to-Type-N<br>from 85054B cal kit<br><u>Pair:</u> Two 7mm-to-<br>Type-N from<br>85054B cal kit |

**E8361A**  
(1.85 mm test ports)

| Equipment Type                       | 1.85 mm                        | 2.4 mm<br>3.5 mm<br>Type-N       |
|--------------------------------------|--------------------------------|----------------------------------|
| Calibration kit<br>or<br>ECAL Module | 85058B<br>N4694A               | See 2.4 mm test port table above |
| Verification kit                     | 85058V                         | See 2.4 mm test port table above |
| RF Cable(s)                          | Single: N4697E<br>Pair: N4697F | See 2.4 mm test port table above |
| Adapters                             | None                           | See 2.4 mm test port table above |

### Cable Substitution

The test port cables specified for the PNA have been characterized for connector repeatability, magnitude and phase stability with flexing, return loss, insertion loss, and aging rate. Since test port cable performance is a significant contributor to the system performance, cables of lower performance will increase the uncertainty of your measurement. It is highly recommended that the test port cables be regularly tested.

If the system verification is performed with a non-Agilent cable, ensure that the cable meets or exceeds the operation of the specified cable. Refer to the cable User's Guide for specifications.



### Calibration Kit Substitution

Non-Agilent calibration kits are not recommended nor supported.

### Precautions for Handling Airlines


When you are using the airlines in the verification kit, observe the following practices to ensure good measurement techniques.

- Be very careful not to drop the airline's center or outer conductor. Damage will result if these devices are dropped.
- Use proper Electro-Static Discharge (ESD) procedures.
- Clean your hands or wear gloves as skin oils will cause a change in electrical performance.

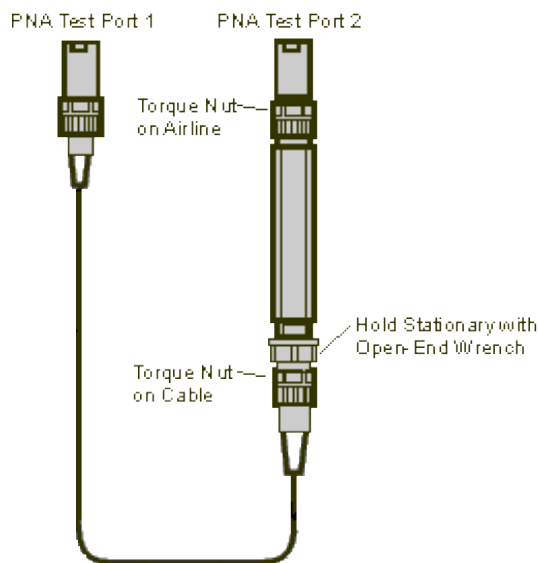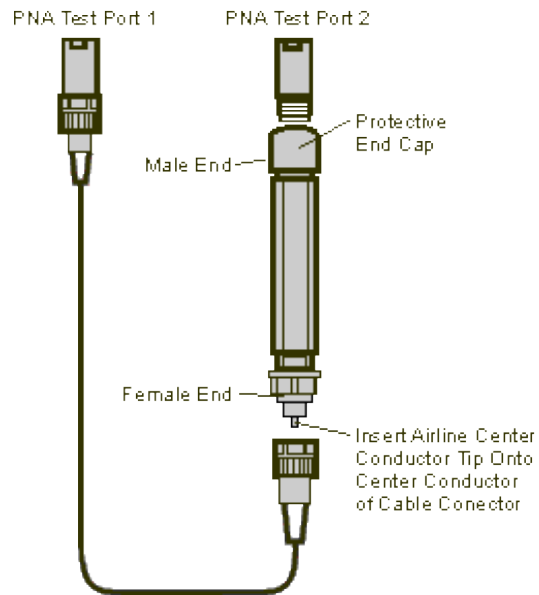

## Flow Diagram of Procedure


The operational flow of the software is depicted by the flowchart shown below.

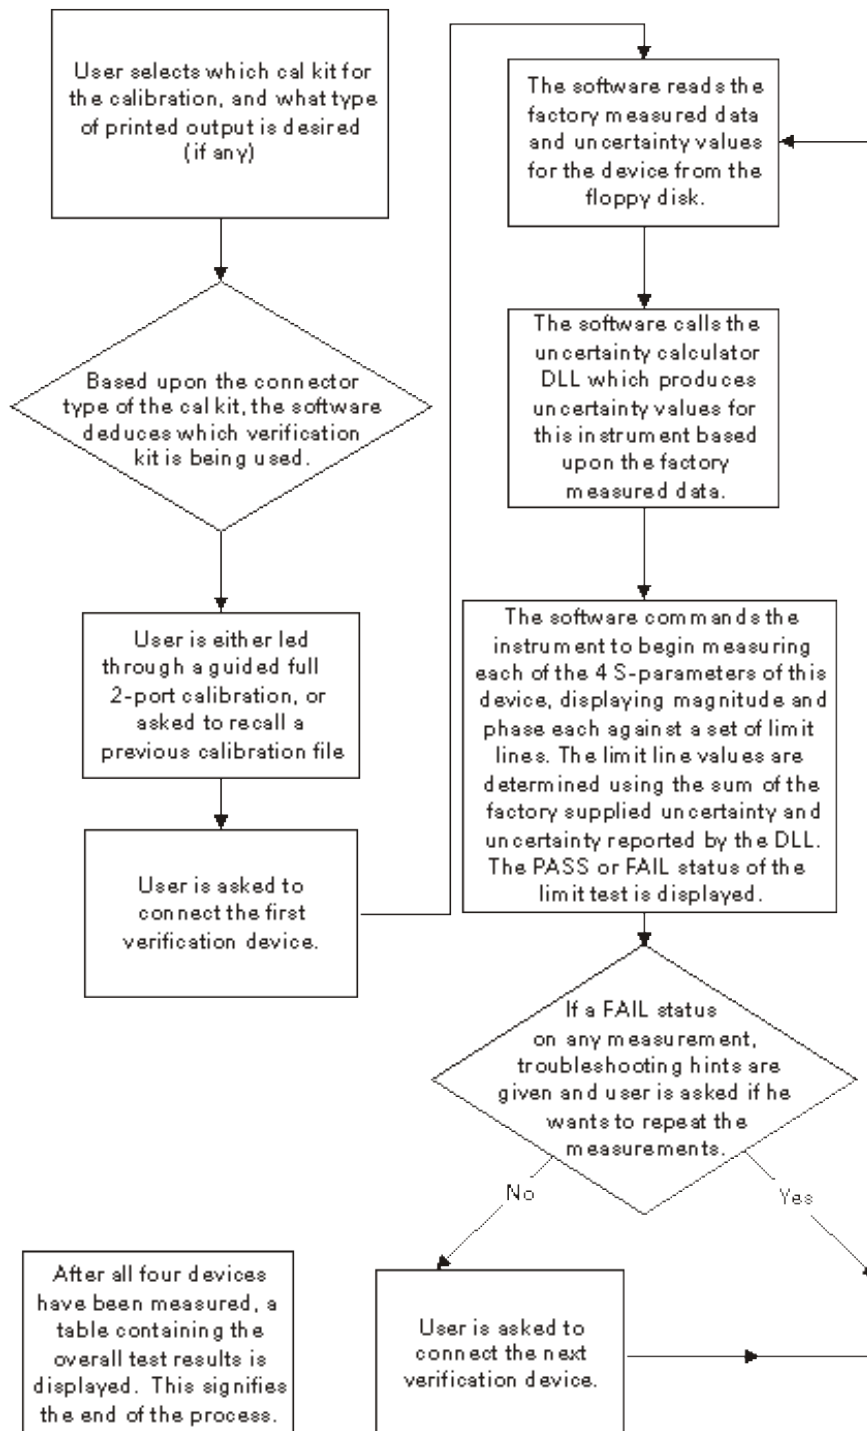

## Procedure for System Verification

1. If you want printed test outputs, connect a printer to the analyzer. Let the analyzer warm up for at least 30 minutes.
2. Insert the PNA verification kit floppy disk into the analyzer disk drive.
3. On the **System** menu, point to **Service**, and click **System Verification**. The System Verification window similar to this will be displayed.

## System Verification window

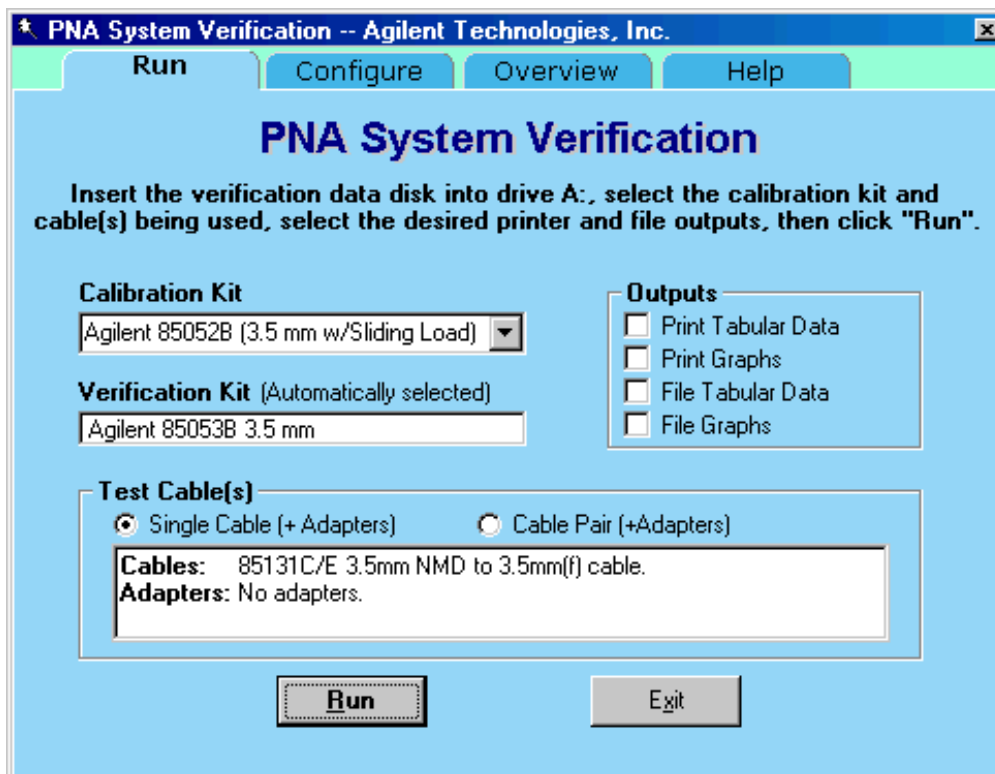

4. In the **Calibration Kit** box, select the calibration kit or ECal module that is being used. The corresponding verification kit to use appears in the **Verification Kit** box.
5. Under **Printer Output** click on any of the following options.
  - **Print Tabular Data:** Prints the verification data in tabular form which includes measured data and uncertainty limits. Refer to a tabular data example, later in this topic.
  - **Print Graphs:** Prints the verification data in graphical form. The graphic form includes the measured data trace, factory supplied data trace and uncertainty limits. Refer to a plot data example, later in this topic.
  - **File Tabular Data:** Writes the verification data in tabular form to a text file in the C:\Program Files\Agilent\Network Analyzer\Documents\ directory.
  - **File Graphs:** Saves a screen image in .PNG format in the C:\Program Files\Agilent\Network Analyzer\Documents\ directory.

---

**Note:** If you want printed output, it is assumed you have already installed the Windows driver for your particular printer, and have tested that you can print to the printer from the network analyzer. This software is designed to print to whichever printer is currently set as the Default printer (see Printers in the Windows Control Panel).

---

6. To modify the number of ports to be verified, to change the number of devices to measure, or to use a previously stored verification calibration, click on the **Configure** tab and make the desired selections.
  - For the system verification to be truly adequate, the software must measure all devices in the kit with a recent calibration applied. Removing and reattaching any test port cables or adapters invalidates all previous calibrations.
7. Click **Run**.
8. Follow the instructions on the analyzer for performing the system verification, inserting the verification

devices as prompted.

---

**Note for 3 Port PNA:**

The System Verification Procedure is **repeated three times**. The first time, **Ports 1 and 2** are measured as a pair; then **Ports 1 and 3** are measured; and lastly, **Ports 2 and 3** are measured.

---

**Note for 4 Port PNA:**

The System Verification Procedure is **repeated two times**. The first time, **Ports 1 and 2** are measured as a pair, then **Ports 3 and 4** are measured.

---

## Step-by-Step Process Description

1. Depending upon the selected choice in the Calibration submenu of the Configure menu, the user is either prompted to recall a previous calibrated instrument state, or is guided through a full 2-port calibration using the selected calibration kit. For ECal, the ECal module is connected just once; a standby message is posted while the software is performing the calibration.
2. The user is prompted to connect the first verification device.
3. The software reads the factory measured data for that device and uncertainty values for that data (CITIfiles) from the floppy disk supplied with the verification kit.
4. The software sends the factory measured data, calibration kit and instrument state information to the uncertainty calculator DLL, which generates uncertainty values specific to the PNA.
5. The analyzer first sets up for magnitude measurements of all four S-parameters, each parameter in a separate window (lin mag for S<sub>11</sub> and S<sub>22</sub>, log mag for S<sub>21</sub> and S<sub>12</sub>). Each of the factory measured S-parameters are fed to the appropriate window as a memory trace. Limit line offsets are calculated as the sum of the factory measured data uncertainties and PNA uncertainties reported by the DLL. Upper and lower limits are displayed (factory measured data + uncertainty sum, factory measured data - uncertainty sum). The PNA takes a sweep, limit test is turned on and PASS/FAIL status is reported in each of the four windows.
6. The user clicks a button when ready to view phase measurements. The four windows get updated for phase format, phase memory traces, phase limits and PASS/FAIL result.
7. If the limit test of any of the four S-parameters (magnitude or phase) indicates a FAIL status, the software suggests troubleshooting tips and asks if the user would like to repeat measurement of that device or proceed to the next device. If proceeding to the next device, the factory measured data and uncertainties for the next device are read from floppy, the uncertainty DLL gets called with this next set of factory measured data, and the four measurement windows get updated for magnitude measurement of the next device.
8. The software follows this same process until all selected devices have been measured, at which point a summary window is displayed containing the set of PASS/FAIL results for all four parameters of each device.


## If the System Fails the Verification Test

**IMPORTANT:** Inspect all connections. Do not remove the cable from the analyzer test port. This will invalidate the calibration that you have done earlier.

1. Repeat this verification test. Make good connections with correct torque specifications for each verification device.
2. Disconnect, clean and reconnect the device that failed the verification test. Then measure the device again.

- If the analyzer still fails the test, check the measurement calibration by viewing the error terms as described in "Front Panel Access to Error Terms" on page 4-7 of the Service Guide.
- Refer to the graphic below, for additional troubleshooting steps.

### Verification Fails Flowchart

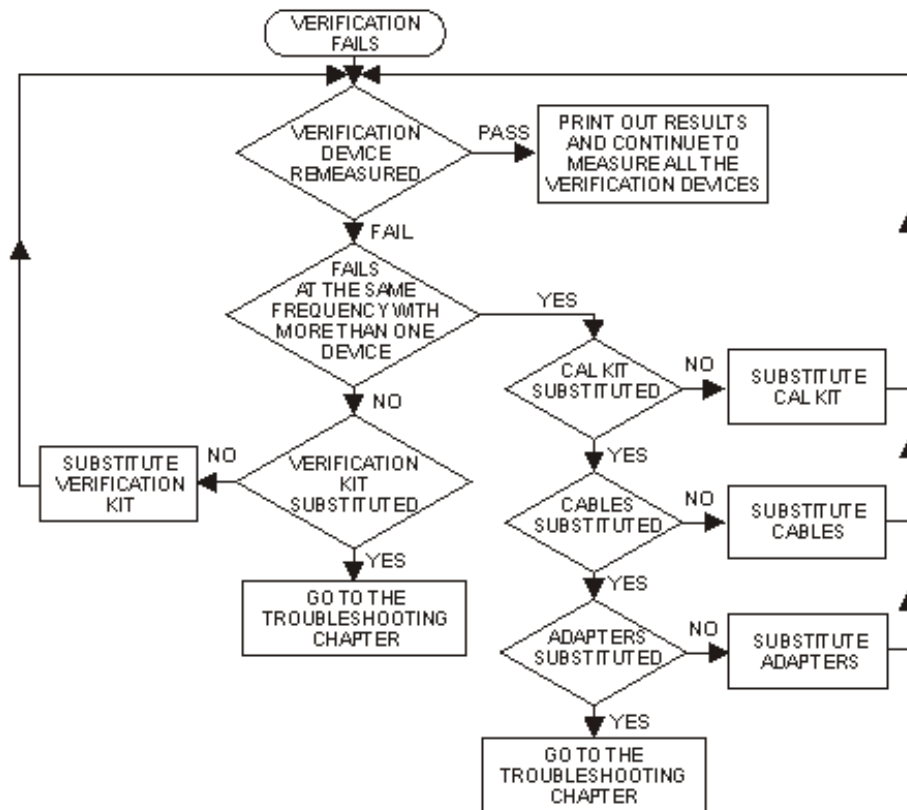

### Interpreting the Verification Results

The graphic below shows an example of typical verification results with **Tabular Data** selected in the **Printer Output** area of the **System Verification** window. A graphic later in this topic shows an example of typical verification results with **Measurement Plots** selected in the **Printer Output** area of the **System Verification** windows. These printouts include a comparison of the data from your measurement results with the traceable data and corresponding uncertainty specifications. Use these printouts to determine whether your measured data falls within the total uncertainty limits at all frequencies.

The tabular data consists of:

- Frequency of the data points (in MHz).
- Lower limit line as defined by the total system uncertainty specification.
- Results of the measurement.
- Upper limit line as defined by the total system uncertainty specification.
- Test status (PASS or FAIL) of that measurement point.

### Printout of Tabular Verification Results







## Source Calibration

---

Source calibration adjusts the PNA source power for flatness across its full frequency range. This adjustment is for service only; not for measurement calibration.

### Required Equipment

Preferred Power Meter: E4419B

Alternate Power Meters: E4419A or EPM-442A

**Note:** The power sensor depends on the PNA frequency range. Depending on the PNA model, two power sensors may be required to test the full frequency range.

The PNA front panel connector type will determine the cable used and if an adapter is required with the power sensor(s).

| PNA Model            | Power Sensor(s)                                                                                                | Cable       |
|----------------------|----------------------------------------------------------------------------------------------------------------|-------------|
| E8356A               | 8482A                                                                                                          | N6314A      |
| E8357A<br>E8358A     | 8482A and E4412A                                                                                               | N6314A      |
| E8801A               | 8482A                                                                                                          | N6314A      |
| E8802A<br>E8803A     | 8482A and E4412A                                                                                               | N6314A      |
| N3381A               | 8482A                                                                                                          | N6314A      |
| N3382A/N3383A        | 8482A and E4412A                                                                                               | N6314A      |
| E8361A               | 8487A (use with adapter 11900B) and<br>V8486A (use with adapter V281B)<br><b>** See E8361A procedure below</b> | N4697-60001 |
| E8362A / B           | E4413A                                                                                                         | 85131E      |
| E8363A/B<br>E8364A/B | 8487A (use with adapter 11900B)                                                                                | 85133E      |

[See PNA Accessories](#)


### Procedure

1. Refer to your power meter documentation to ensure the proper calibration factors for the power sensor have been entered into the table on the power meter.
2. Connect a GPIB cable between the power meter and network analyzer.
3. Ensure the power sensor(s) are connected to the power meter.
4. In the analyzer **System** menu, point to **Service, Adjustments**, and click **Source Calibration**.

5. The software presents you with three choices:

- a. Click **Inspect Linearity** to observe how accurately the power steps from one power level to the next. When finished, Test Output Power Linearity should meet specification for your PNA Model.
- b. Click **Inspect Amplitude** to observe flatness of the source power versus frequency for three power levels: -5 dBm, 0 dBm and +5 dBm. When finished, Test Output Power Accuracy should meet specification for your PNA Model.
- c. Click **Calibrate** to begin the source calibration process. The software begins by identifying the power meter and sensor. Then you are prompted to connect the sensor(s) and cable as needed.

### Connecting sensors to the PNA

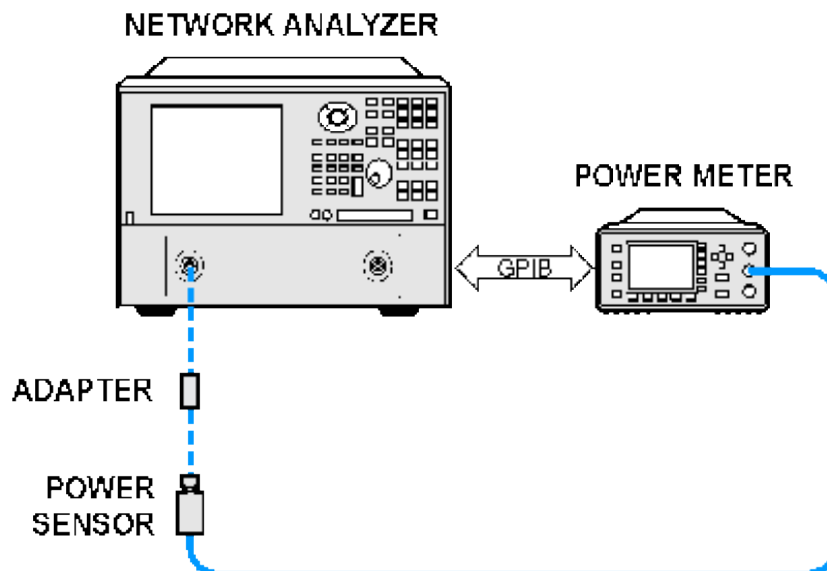

### Additional Information

All ports are tested on all PNAs. Source calibration takes approximately 20 to 90 minutes to complete depending on the frequency range of the PNA.

### Troubleshooting

In the event there is a problem with Source Calibration, please refer to the "Troubleshooting" chapter in the PNA Service Guide.

### E8361A Procedure

Source and Receiver calibration requires the power meter to measure the source power over the full range of each of the PNA internal bands. Because the 8487A can not measure accurately above 50 GHz, it can only be used up to the next highest band switch frequency at 46.2 GHz. The V8486A sensor and V281B adapter are used from 46.2 GHz to 67 GHz.

For highest accuracy, the V8486A and V281B should be sent to Agilent for a custom calibration from 45 GHz to 70 GHz.

For the next highest accuracy level, the following procedure shows how to measure correction factors yourself from 46 to 50 GHz. This procedure assumes you have already loaded correction factors for both sensors into the power meter.

1. On your power meter, add 46 and 48 GHz to the Cal Factor Table.
2. Preset the PNA
3. Tune the PNA to 46 GHz (CW frequency)
4. Using the 8487A, measure power at port 1. Record this value.
5. Tune the PNA to 48 GHz (CW frequency)
6. Using the 8487A, measure power at port 1. Record this value.
7. Connect the V8486A, V281A, and 1.85 f-f adapter to the power meter.
8. Tune the PNA to 46 GHz (CW frequency)
9. Adjust the cal factor table 46 GHz setting until the power meter reading matches the power readings from step 4.
10. Tune the PNA to 48 GHz (CW frequency)
11. Adjust the cal factor table 48 GHz setting until the power meter reading matches the power readings from step 8.

## Receiver Calibration

---

Receiver calibration adjusts the network analyzer receivers for a flat response across its full frequency range. This adjustment is for service only; not for measurement calibration.

### Required Equipment

Preferred Power Meter: E4419B

Alternate Power Meters: E4419A or EPM-442A

**Note:** The power sensor depends on the PNA frequency range. Depending on the PNA model, two power sensors may be required to test the full frequency range.

The PNA front panel connector type will determine the cable used and if an adapter is required with the power sensor(s).

| PNA Model            | Power Sensor(s)                                                                                                       | Cable       |
|----------------------|-----------------------------------------------------------------------------------------------------------------------|-------------|
| E8356A               | 8482A                                                                                                                 | N6314A      |
| E8357A/E8358A        | 8482A and E4412A                                                                                                      | N6314A      |
| E8801A               | 8482A                                                                                                                 | N6314A      |
| E8802A/E8803A        | 8482A and E4412A                                                                                                      | N6314A      |
| N3381A               | 8482A                                                                                                                 | N6314A      |
| N3382A/N3383A        | 8482A and E4412A                                                                                                      | N6314A      |
| E8361A               | 8487A (use with adapter 11900B) and V8486A (use with adapter V281B)<br><b>** See <a href="#">E8361A procedure</a></b> | N4697-60001 |
| E8362A / B           | E4413A                                                                                                                | 85131E      |
| E8363A/B<br>E8364A/B | 8487A (use with adapter 11900B)                                                                                       | 85133E      |


See [PNA Accessories](#)

### Procedure


1. Refer to your power meter documentation to ensure the proper calibration factors for the power sensor have been entered into a table on the power meter.
2. Connect a GPIB cable between the power meter and network analyzer.
3. Ensure the power sensor(s) are connected to the power meter.
4. In the analyzer **System** menu, point to **Service, Adjustments**, and click **Receiver Calibration**.
5. The software presents you with two choices:

- a. Click **Inspect Flatness** to observe flatness of receiver response versus frequency. Although there is no explicit specification for receiver flatness, Receiver Calibration should improve Transmission and Reflection Tracking error terms which are specified.
- b. Click **Calibrate** to begin the receiver calibration process. The software prompts you to connect the sensor(s), cable and adapter as needed (see the following graphics).

### Connecting sensor(s) to the PNA

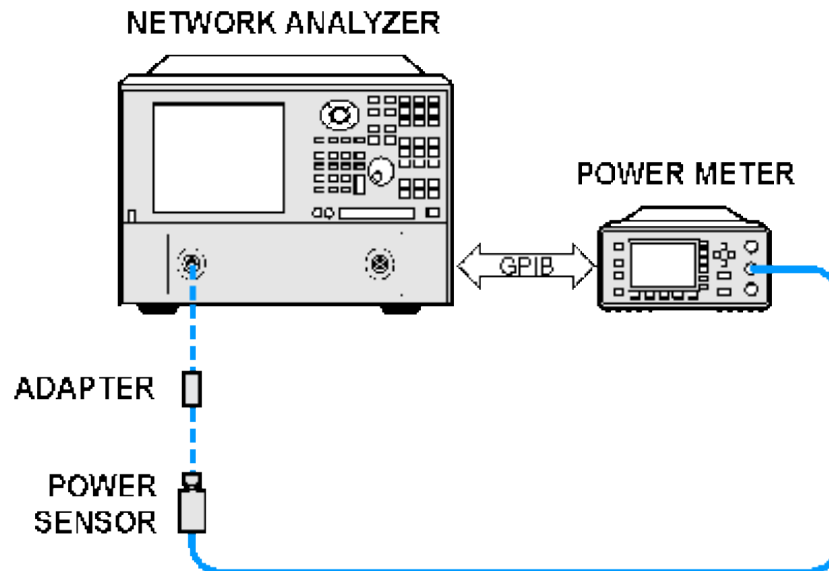


### Connecting adapter and cable between sensor and PNA

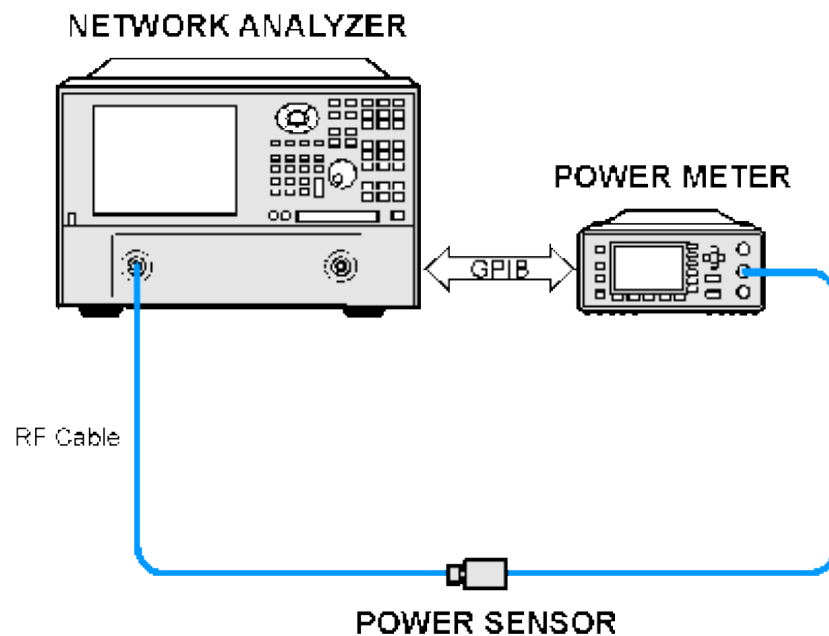

### Through connection using the specified cable

## NETWORK ANALYZER

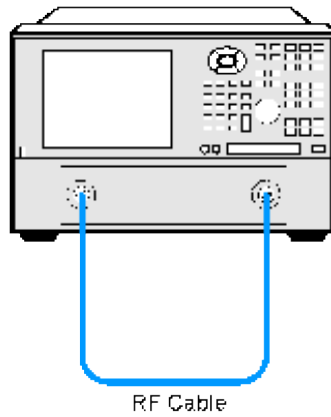

### **Additional Information**

Receiver Calibration tests all PNA receivers, taking approximately 15 and 45 minutes. Length is dependent on frequency range and number of ports.

### **Troubleshooting**

In the event there is a problem with Receiver Calibration, please refer to the "Troubleshooting" chapter in the Network Analyzer Service Guide.



## Receiver Display

---

### The Receiver Display as a Troubleshooting Tool

#### How to start the Receiver Display


#### Other Support Topics

### The Receiver Display as a Troubleshooting Tool

The Receiver Display is a Troubleshooting Tool. It enables the analyzer to isolate faulty functional groups within its own Measurement System. Traces for each Receiver are Displayed in individual windows. Identifying discrepancies of the traces in these windows can help isolate the faulty assembly.

For a thorough description of Receiver Display and the troubleshooting steps see Chapter 3 of the PNA Service Guide. You can download the Service Guide for your PNA model from our website: <http://www.agilent.com>.

#### How to Start the Receiver Display

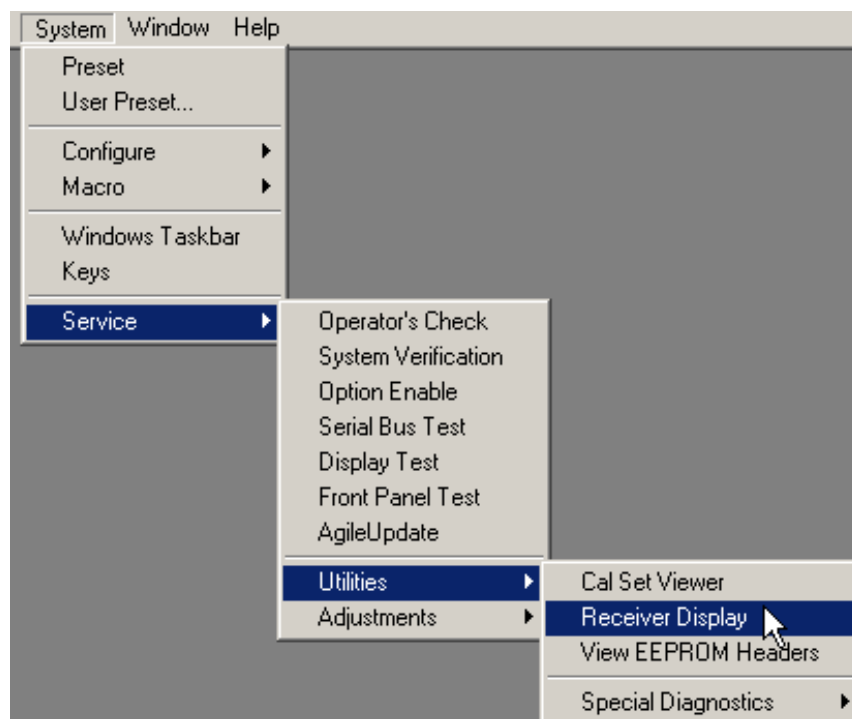

Learn more about using the [front panel interface](#)

## Serial Bus Test

---

This test is designed to work with the PNA Series Network Analyzer as it was originally manufactured. If any of the following assemblies have been replaced in the analyzer, this test may not show accurate pass/fail results.


- A8
- A10
- A11
- A12

This test sequentially tests all 32 nodes at 300 kHz, and then all nodes whose values change with frequency, at 11 other frequencies. All measured values are written to an ASCII text file in the service directory any measured values which exceeded their tolerances are highlighted in the application and the data file.

The assemblies tested and their associated node numbers are as follows:

| Board Assembly              | Node Numbers |
|-----------------------------|--------------|
| A12 Source Assembly         | 111 to 118   |
| A10 Frequency Reference     | 211 to 218   |
| A11 Phase Lock              | 311 to 318   |
| A8 Fractional-N Synthesizer | 411 to 418   |

### How to Start Serial Bus Test

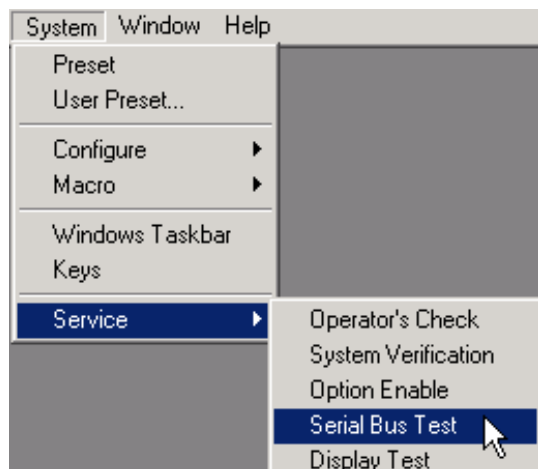

Learn more about using the [front panel interface](#)

---

**Note:** If any errors are reported, refer to the service guide.

## Instrument Calibration

---

An instrument calibration is a process where the analyzer performance is measured to ensure that the analyzer operates within specifications. If any performance parameter does not conform to the published specifications, adjustments are made to bring the performance into conformance.

### Why Should I Get an Instrument Calibrated?

Over time, the active components in the analyzer age and the performance may degrade or drift. To ensure that the analyzer is performing to the published specifications, you must have an instrument calibration performed periodically.

### How Often Should I Get an Instrument Calibrated?

The instrument specifications are set to consider the performance drift that may occur over a 12 month period. Therefore, getting the instrument calibrated at 12 month intervals ensures that the analyzer maintains performance within the operating specifications. If you need the analyzer to maintain more consistent operation parameters, you may want to have the instrument calibrated more often than the suggested 12-month interval.

### How Do I Get an Instrument Calibrated?

To get the instrument calibrated, send it to one of the Agilent Technologies service centers. See Technical Support.


The PNA must be fully functional when it is sent to the service center, or they will charge for their repair services. If the PNA is being used in a secure environment where the hard drive can not be sent with the PNA, a second hard drive must be purchased and configured for use with the PNA in an "unclassified" environment before the PNA is sent to the service center.

To perform the instrument calibration yourself, you must have the following required items:

- Instrument Calibration Test Equipment
- Performance Test Software

### What Are My Choices of Instrument Calibration?

The following types of instrument calibration are available from Agilent Technologies:

|                                                                                                        |                                                                                                                                                                                                              |
|--------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Standard</b><br> | Includes a certificate of calibration, stating the instrument has been calibrated and is operating within the published specifications.                                                                      |
| <b>Option UK6</b>                                                                                      | Includes the test data from the calibration and the standard certificate, stating the instrument has been calibrated and is operating within the published specifications.                                   |
| <b>Option M40 (Special)</b>                                                                            | Includes the test data from the calibration and a certificate, stating the instrument has been calibrated using a process in compliance with ANSI Z540 and is operating within the published specifications. |

### Other Support Topics

## About IF Access (H11 Option)

The PNA H11 option provides rear panel access to the PNA IF paths. You can also set the gain of the IF amplifiers.

See if your PNA can be [upgraded to the H11 option](#).

### [How to Make IF Access Settings](#)


#### [IF Gain Configuration](#)

#### [IF Switch Configuration](#)

### Other IF Access Topics

### [N5250A Typical System Performance](#)


#### How to Make IF Access Settings

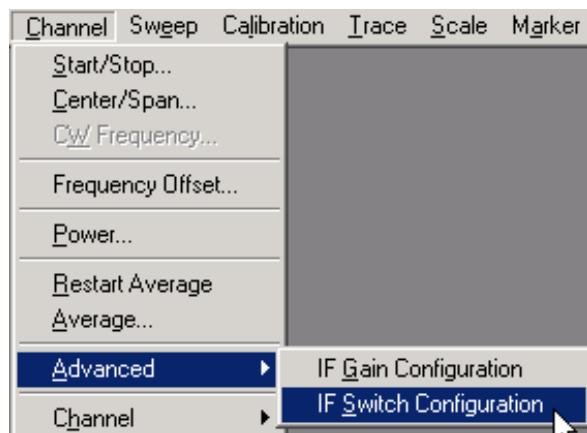

Learn more about using the [front panel interface](#)

## IF Gain Configuration

The IF Gain Configuration settings allow you to manually set the gain of the PNA IF amplifiers.

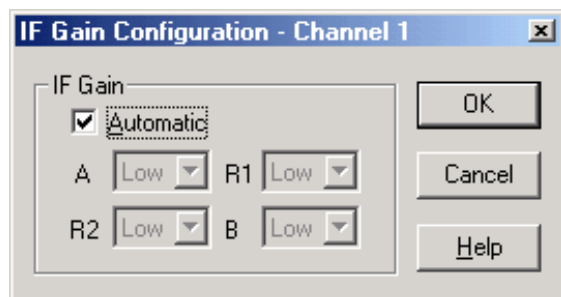

## IF Gain Configuration dialog box help

**Automatic** - check to allow the PNA to set the IF gain automatically. Clear to enable manual IF gain settings.

**Note:** Clearing the **Automatic** checkbox can result in inaccurate measurements.

**A, R1, R2, B Receivers**

**Auto Gain** - The PNA selects the best gain level to make pulsed measurements.


Low - about 0 dB of gain

Med - about 17 dB of gain

Hi - about 34 dB of gain

## IF Switch Configuration

The IF Switch Configuration settings allow you to select the input path to the PNA IF amplifiers.

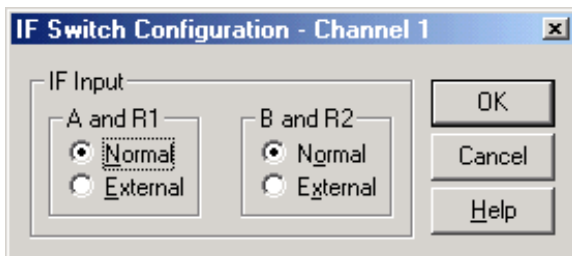

## IF Switch Configuration dialog box help

Available only with the H11 option

**Normal** - allow the PNA to decide the input path to the PNA IF amplifiers.

**External** - always use the rear panel inputs to the PNA IF amplifiers.

## External Millimeter Module Configuration

---

You can use external Millimeter Modules to extend the frequency coverage of your PNA. To use this feature your PNA must have the [H11 Option](#).

### [PNA Limitations when using External Millimeter Modules](#)

### [How to Configure Millimeter Modules](#)


#### Other IF Access Topics

### PNA Limitations when using External Millimeter Modules


**Power Settings** When using external Millimeter Modules, the PNA cannot control the power level into your DUT above 67 GHz. Because of this limitation, PNA power settings will not function correctly. Some of these settings are: Power level in standard or segment sweep, source and receiver power calibrations, and calibration interpolation. Your modules may have a manual power control.

**Frequency Offset Measurements** Because of the many configurations used in frequency offset, we do not support Frequency Offset measurements when using external Millimeter Modules.

#### How to Configure Millimeter Modules

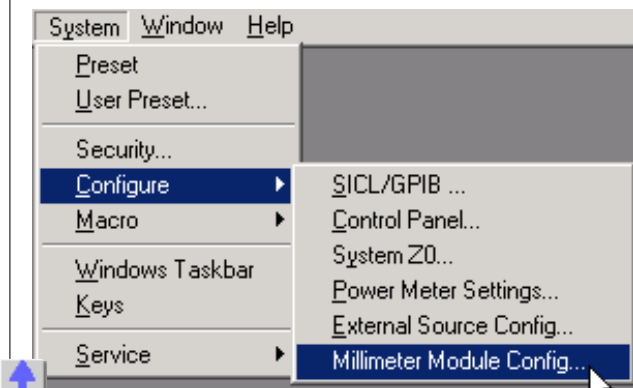

Learn more about using the [front panel interface](#)

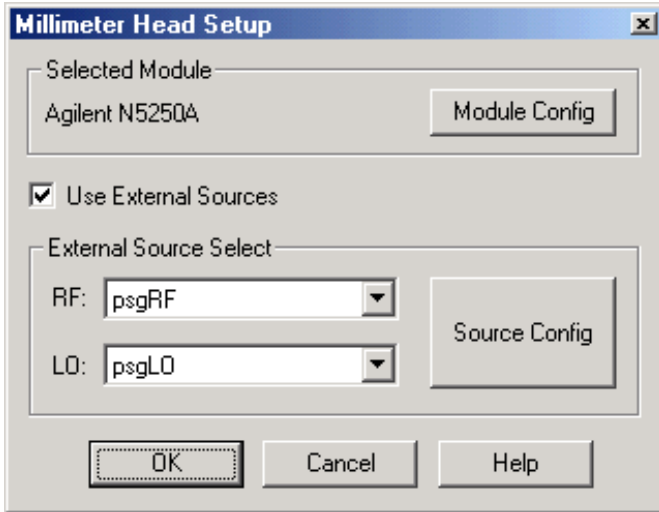

## Millimeter Head Setup dialog box help

### Important Notes

- The External Sources will become UNSYNCHRONIZED after performing an Instrument Preset, recalling an instrument state, or adding a Channel. When this occurs, launch this dialog box again and click **OK**. We strongly recommend using only one channel to make measurements using external sources.
- For measurements up to 110 GHz, the amount of phase noise is comparable when using either the internal PNA sources or external sources. For the best measurement accuracy at frequencies above 110 GHz, it is strongly recommended that external sources be used.
- Only Agilent PSG sources are supported.


**Selected Module** Displays the currently selected module. To select and configure a different module, click Module Config.

**Use External Sources** Check to use external sources to provide an LO for the Millimeter Modules.

**Source Config** Click to invoke the External Source Configuration dialog box. This dialog box is also used to configure external sources for the FCA application. Ignore references to FCA in the help topic.

In addition, the following settings on that dialog box are NOT relevant for Millimeter Head Setup:

- **Trigger Mode** Hardware List (BNC) triggering is always used to control the RF and LO sources for Millimeter Wave Heads. Read the notes and follow the setup diagram for two external sources.
- **LO Calibration** The power out of the sources is set and controlled by the PNA H11 option.

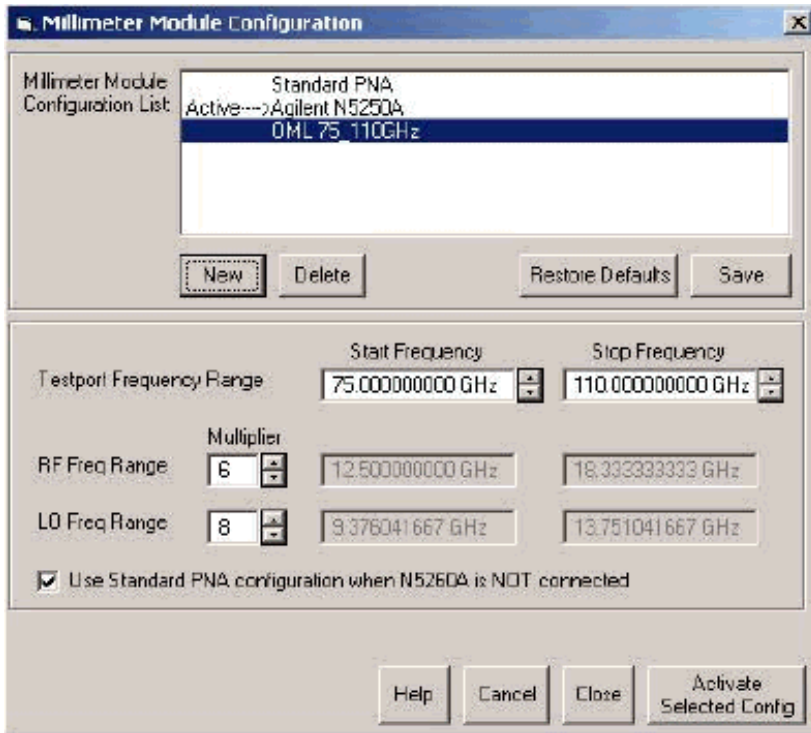

## Millimeter Module Configuration dialog box help

**Millimeter Module Configuration List** Lists the standard PNA configuration and others that you have created.

**New** Click to create a new Millimeter Module Configuration. Invokes the **Name** dialog box. Type a unique name for the new configuration using only alphanumeric characters and underscore, then click OK.

**Delete** Remove a Millimeter Module Configuration.

**Restore Defaults** Prompts, then REMOVES all configurations except for the standard PNA (and N5250A if installed).

**Save** Saves the current settings to the PNA hard drive.

**Testport Frequency Range** Set the Start and Stop frequencies of the selected configuration at the test ports. When Activated (click **Activate Selected Config**), this becomes the displayed Start and Stop frequency of the PNA.

**RF Freq Range Multiplier** RF Frequency Range (displayed in grey fields) multiplied by this value = Testport Frequency Range.

Use the Multiplier values that are specified in your test head documentation.

**LO Freq Range Multiplier** LO Frequency Range (displayed in grey field) multiplied by this value + 8.33 MHz = Testport Frequency Range.

**Note:** If the LO and RF frequency ranges are not within the operating range of the PNA, a warning message appears along with a red box around the invalid field. Click the appropriate Multiplier value up or down to correct the problem.

**Use Standard PNA operation when N5260A is NOT connected** When Activate Selected Config is clicked, the PNA detects if a N5260A is connected. If one is NOT connected and:

- This box is checked, then the selected configuration is NOT activated, but uses the Standard PNA configuration.



- This box is cleared, then the selected configuration IS activated anyhow.

**Cancel** Closes dialog box without saving changes.

**Close** Prompts to save changes, then closes the dialog box.

**Activate Selected Config** Saves the configuration, then closes and restarts the PNA application with the new configuration. To change to another configuration, including the standard PNA configuration, you must make this selection again.

## Pulsed Application

The Pulsed Application is a Visual Basic program that provides a user interface for making pulsed measurements.

### [Required Options](#)

### [Using the Pulsed Application](#)

### [How to Configure Pulse Generators and Receivers](#)

### [Pulse Profiling](#)

### [Signal Reduction versus Gate Width](#)

### [Pulsed Frequency Converter Measurements](#)

### [Writing your own Pulsed Application](#)

For more conceptual information on pulsed measurements, visit [www.Agilent.com](http://www.Agilent.com) and search for **AN 1408-11**.



## Other IF Access Topics

### Required Options


The PNA H08 option provides the Pulsed Application. The H08 option requires that your PNA also have [Opt 014 \(front panel access\)](#) and [Opt 080 \(frequency offset\)](#). To use the internal receiver gating feature of the Pulsed Application, your PNA must have the [H11 hardware option](#). If your PNA does not have the required options, a message is displayed on the screen.

### Using the Pulsed Application

#### How to start the Pulsed Application

1. Press  until **Pulse** is visible, then 

or

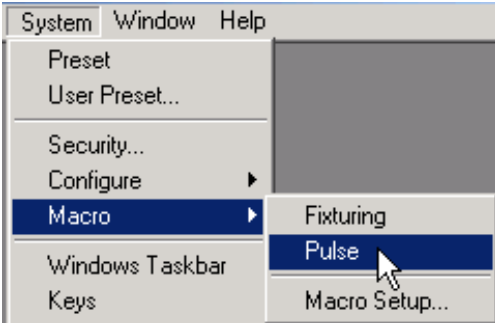
2. 

Learn more about using the [front panel interface](#)

### Keypad Data Entry

The PNA Numeric Entry and Navigation keys can be used for dialog box input. Also, a keyboard can be used to enter values, including alpha characters for prefixes (for example, **u** for usec.) . After typing values, first press **Enter**, then press **Tab** to go to the next field.

The following is an image of the main dialog box:

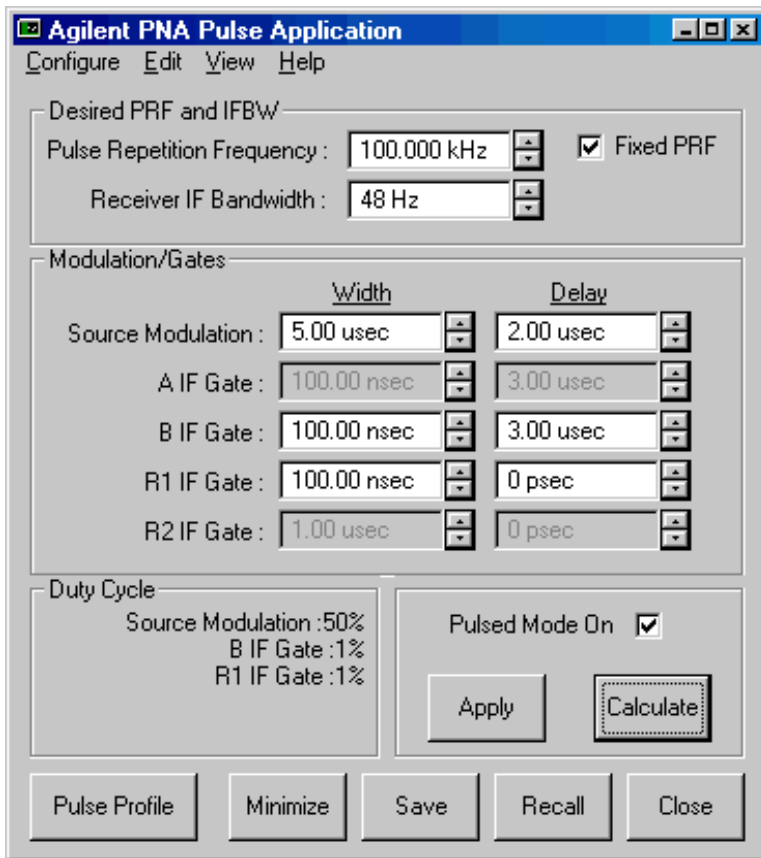

### Pulsed Application Main dialog box help

**Note:** An **error message** may appear on the PNA stating that the response frequency has exceeded the maximum allowed frequency.

The pulsed application may set the offset frequency (option 080) of the PNA to some value other than zero (the default value). If the stop frequency is set to the maximum of the PNA model, then the error message will appear.

To fix this, set the stop frequency to a value that is at least 2 KHz less than the maximum allowed. For example, if you have a 20 GHz PNA, and the stop frequency is set to 20 GHz, and the error message appears, then set the stop frequency to 19.999998 GHz

### Configure

You can configure more than one channel to make pulsed measurements, but the channels must use the same pulse generator settings.

Only the Agilent 81110A Pulse Generator is supported with the Pulsed Application. Refer to the 81110A documentation for pulse repetition frequency and duty cycle capabilities.

See also:

[Configure Receivers](#)

[Converter Measurements](#)

**Edit / Undo** Pulse Application settings revert to those when Apply was last pressed.

**Desired PRF and IFBW** Enter the DESIRED values. When **Calculate** is pressed, one or both of these values may change.

**Pulse Repetition Frequency:** Frequency of the pulses from the Pulse Generator.


**Receiver IF Bandwidth:** IF Bandwidth of the PNA. Choose a setting from 1 Hz to 10 KHz.

**Fixed PRF** When checked, (default setting) the **Calculate** algorithm will NOT adjust the PRF, but only change the IF Bandwidth.

**Modulation/Gates** The Source Modulation and four PNA receiver gates can each have their own, or share, Pulse Generator outputs. Shared outputs have identical Width and Delay values. To configure and enable outputs, click **Configure**, then **Pulse Generators** to launch the Pulsed Generator Configuration dialog box.

**Width** Pulse Width.

**Delay** The delay that occurs before the pulse.

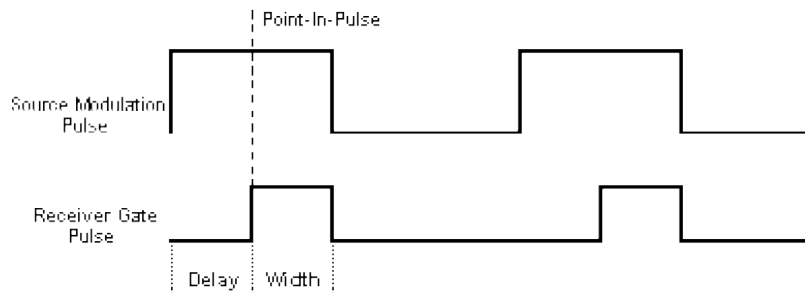

**Duty Cycle** Calculated Duty Cycle of the source and each of the selected receivers.

**Pulse Mode On** When this box is checked, the PNA is enabled for Pulsed measurements. The PNA Status Bar annotation indicates the following:

- **G** Internal IF gates enabled.
- **F** Filtering for Pulsed Measurements enabled.

**Apply** All selections are sent to the pulse generator and the active channel of the PNA.

**Calculate** All selections are calculated and valid PRF and IFBW values are entered in their fields. If these settings are not acceptable, try changing the values you previously entered and click Calculate again. When acceptable values are attained, click Apply to send these values to the pulse generator and PNA.

**Pulse Profile** Launches the Pulse Profile dialog box. Same as clicking **View / Pulse Profile**.

**Minimize** Click to minimize the dialog box to make changes in the PNA application.


**Save** All settings from the Pulsed Application are saved in a \*.ppf file. These settings are NOT saved with PNA instrument state.

**Recall** Restore settings from the specified \*.ppf file that were previously saved.


**Close** Closes the dialog box without saving changes.

## How to configure Pulse Generators and Receivers

From the Pulse App main dialog box



If this setting is unavailable, click Calculate.

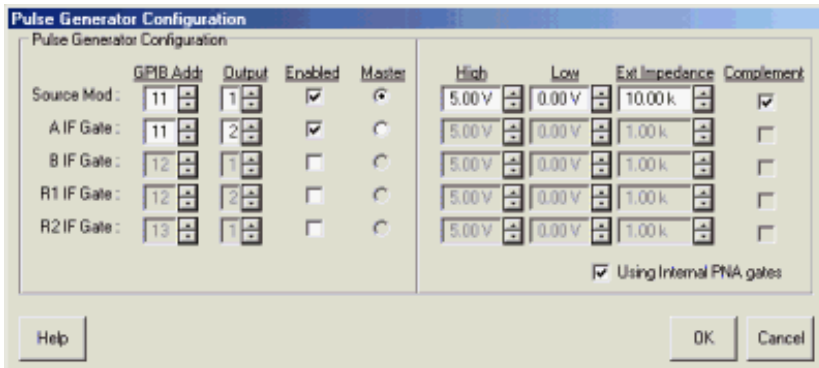

## Pulsed Generator Configuration dialog box help

Configures the Agilent 81110A Pulse Generator outputs. You can configure each 81110A Pulse Generator with either one or two 81111A output modules.

The Source Mod and four PNA receiver gates can each have their own, or share, pulsed outputs. To share a generator output between one or more PNA inputs, use the same GPIB address and output module for each PNA input. This causes the shared PNA inputs to have identical **Width** and **Delay** values selected on the Main dialog.

**Source Mod:** The output that pulses the PNA source.

**A, B, R1, R2 IF Gate:** The PNA rear panel connector to receive the gating pulse.

**GPIB Addr:** The GPIB address of the 81110A.

**Output:** The output module of the 81110A.

**Master:** The 81110A that uses the 10 MHz reference signal from the PNA.

**Enabled:** Turns the pulse output ON.


**High:** Specify a 'TTL-High' voltage level

**Low:** Specify a 'TTL-Low' voltage level

**Ext Impedance:** Impedance of the DUT

**Complement:** When this box is cleared, TTL HIGH is the pulse. When checked, TTL LOW is the pulse.

**Using Internal PNA gates** When this box is checked, the voltage, impedance, and complement values are forced to settings that prevent damage to the internal gates.

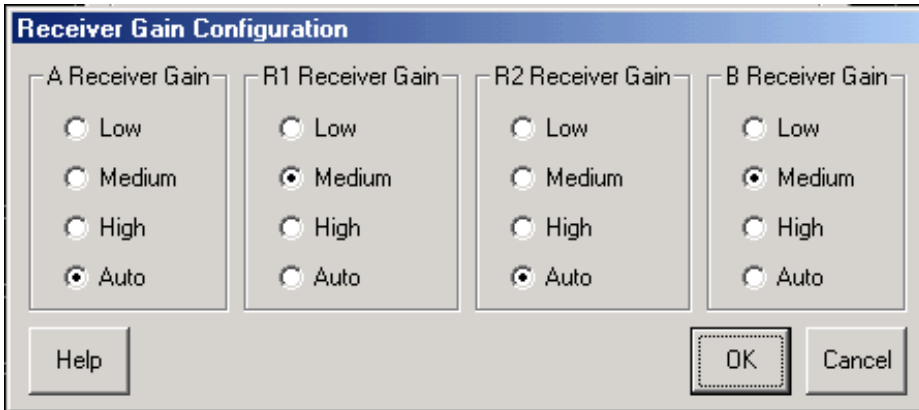

### Receiver Gain Configuration dialog box help

Sets the gain of each receiver manually or automatically.

**Auto** - The PNA selects the best gain level to make pulsed measurements.

Use these to manually set the gain for each receiver.

**Low** - about 0 dB of gain

**Medium** - about 17 dB of gain

**High** - about 24 dB of gain

Some PNA models have only two gain settings instead of three as in the previous graphic.

## Pulse Profiling


Pulse profiling provides a time domain view of the pulse envelope. Profiling is performed using a measurement technique that "walks" a narrow receiver "snapshot" across the width of the pulse. This is analogous to using a camera to take many small snapshots of a wide image, then piecing them together to form a single, panoramic view.


- Pulse Profiling can be performed using ratioed or unratioed measurements.
- Pulse Profiling is performed at a single CW frequency.

### How to perform Pulse Profiling

From the Pulse App main dialog box

If this setting is unavailable, click Calculate.



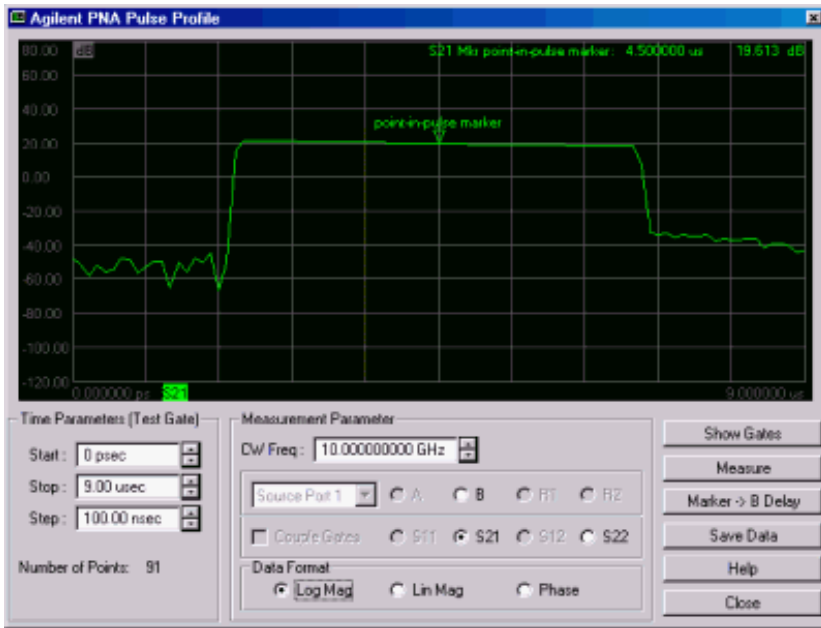

## Pulse Profile dialog box help

[Learn about Pulse Profiling \(scroll up\)](#)

### Time Parameters

**Start, Stop** These two combine to make the window of the assembled pulse profile. To view the entire pulse, the start and stop values must be at least as wide as the Source Modulation Width plus Delay value (from the main [Pulse App dialog box](#)).

**Step** Each consecutive snapshot is incremented by this value until the stop value is reached. Therefore, the number of points for the pulse profile measurement can be calculated as:  $(\text{Stop} - \text{Start}) / \text{Step}$ . The higher the number of points, the longer it takes to make the measurement.

### Measurement Parameter

**CW Freq.** Frequency of the PNA source.

**Source Port** The PNA port supplying the source power for single receiver measurements (Receivers A, B, R1, R2)

**Select a Measurement** Only those receiver gates that are configured in [Pulsed Generator Configuration](#) are available. Select from the following:

**Unratioed (single receiver) - A, B, R1, R2**

OR

**S-parameters (ratioed)**


Measurements that are available depend on which receiver gates are [configured](#):

- To measure S11, configure A and (optionally) R1.
- To measure S21, configure B and (optionally) R1.
- To measure S12, configure A and (optionally) R2.
- To measure S22, configure B and (optionally) R2.

If the reference receiver gate (R1 or R2) is NOT configured, the average of the Source Modulation pulse is used as the reference.

**For example:**

**S21 Selected, ONLY B receiver gate is configured**

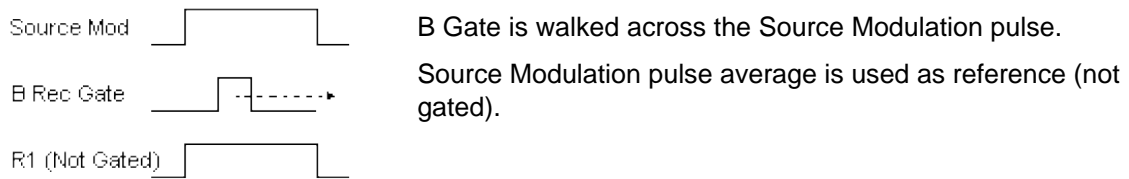


**Coupled Gates** Available when the appropriate receiver gates are configured for your ratioed measurement.

- **Uncoupled** (box cleared) The reference gate is FIXED at the delay setting as the test gate is walked across the Source Modulation pulse.

**For example:**

**S21 Selected, B and R1 receiver gates configured, Gates Uncoupled**

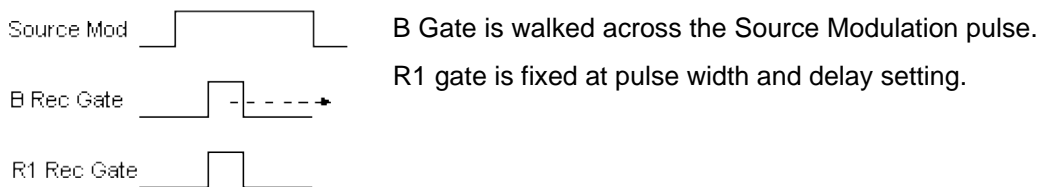


- **Coupled** (box checked) The reference gate is walked simultaneously with the test gate at the specified delay values.

**For example:**

**S21 Selected, B and R1 receiver gates configured, Gates Coupled**

**B gate delay = 3 microseconds, R1 gate delay = 2 microseconds,**

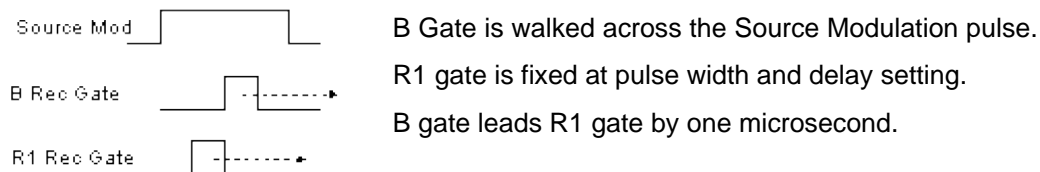

**Data Format** Log Magnitude, Linear Magnitude, or Phase (only available if S-parameter selected).

**Buttons**

**Show Gates** Allows you do change the receiver gating width and delay while looking at the results.

**Measure** Click to start the pulse profile measurement. A bar above the button indicates progress.

**Marker to Delay** After making a measurement, you can drag the display maker to any point along the trace. Click this button and the marker time is entered into the Receiver **Delay** field on the main dialog box.

**Save Data** Saves time domain data to the PNA hard drive in any of the following formats:



- Touchstone (\*.s1p)
- Comma delimited (\*.prn)
- Citifile (\*.cti)


[Learn more about these data formats.](#)

## Signal Reduction versus Gate Width


### Signal Reduction versus Gate Width

PRF = 1 MHz

The following two figures show the performance of the internal IF gates as the width is narrowed.

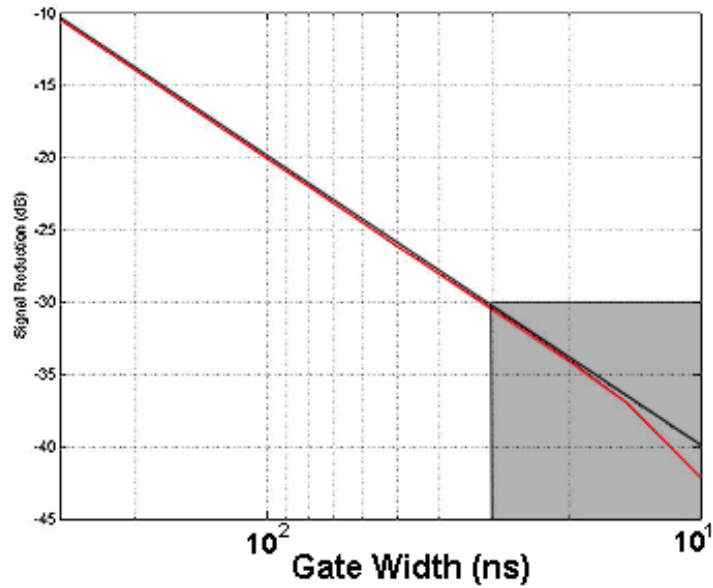

The following is a zoomed image of the shaded area (above).

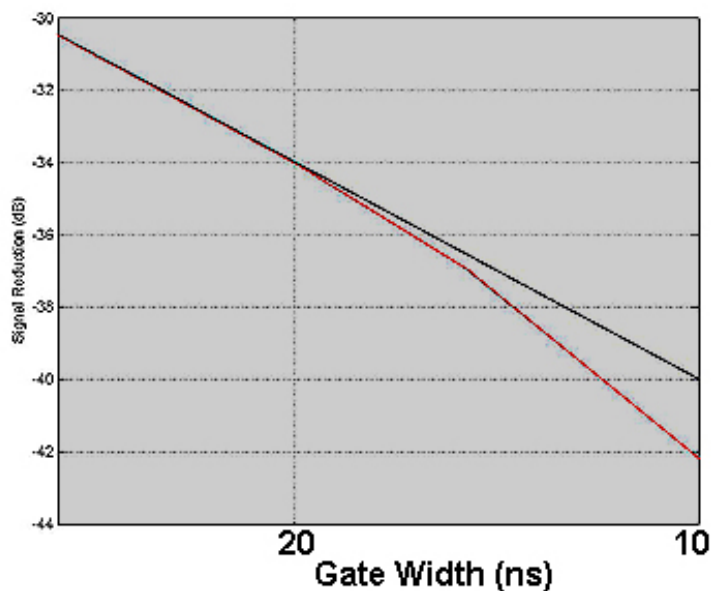


- The straight line shows the theoretical loss in dynamic range due to duty cycle effects when using narrowband detection.
- The curved (red) line shows the actual measured performance of the gates.
- The minimum gate width for <1dB deviation from theoretical is approximately 20ns.

See the specifications for the [option H11](#) and [option H08](#).

## Pulsed Frequency Converter Measurements

The Pulsed Application works with both [FCA \(option 083\)](#) and standard [Frequency Offset \(opt 080\)](#) measurements. On the **Configure** menu, check **Converter Measurements**. When checked, this setting prevents the Pulsed Application from [overwriting frequency offset values](#). This may limit the number of **PRF** and **IFBW** solutions that are returned when **Calculate** is pressed on the main Pulsed Application dialog box.

**Note:** Pulse Profiling can NOT be performed with frequency converter measurements.

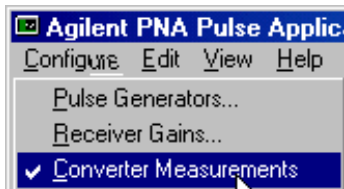

## Writing your own Pulsed Application

You can use the Pulsed Application or use the [example program](#) as a template for making your own Pulsed Application.

The Pulsed Application uses a custom .dll to perform the calculations that are necessary to make pulsed measurements. Use the [ConfigNarrowBand3 Method](#) to send and return values to **agilentpnapulsed.dll**. Then use [SCPI](#) or [COM](#) commands to control the PNA.

## Install and Register the Pulsed .dll on your PC

To create your own Pulsed Application, or run the Pulsed Application from a remote PC, you must do the following:

1. Copy the following files from the PNA `C:\program files\agilent\network analyzer\` to a directory on your PC.

- **agilentpnapulsed.dll**
- **OffsetList.txt**
- **prfbw.txt**
- **prfbwmixer.txt**

2. To register the ActiveX DLL in Microsoft Windows Operating System:

- From a command prompt on your PC, navigate to the directory where you copied the DLL.
- Type: **regsvr32 agilentpnapulsed.dll** and press **Enter**

For Operating Systems other than Windows, see their associated help files to learn how to register DLL files.

## E5091A Testset Control

---

The E5091A is a popular Agilent Technologies 7-port / 9-port testset. Although the testset was originally designed to work with the ENA Network Analyzer, it also works well with the PNA. This topic describes how to control the testset from the PNA. For more information about the testset, refer to your E5091A documentation.

### [Overview](#)

### [Connecting the E5091A](#)

### [How to make E5091A Testset Control Settings](#)

### [Calibrating with the E5091A](#)

## Other Setup Measurements Topics

### Overview

When connected to the PNA, the E5091A Testset provides full 7-port or 9-port test capability. The E5091A can be configured to switch a different testset path for each PNA channel. When all channels have been configured, the entire measurement setup and calibration can be [saved to a .cst or .csa file](#) to be recalled later. In addition, the [Channel Settings Table](#) that is appended to a printed hardcopy of a measurement includes the E5091A Port Control settings.

#### Notes:

- The E5091A Testset has a maximum useful frequency of 11 GHz.
- The E5091A Testset Control can be automated using [SCPI](#) and [COM](#) commands.
- When [enabled](#), a second status bar row appears which indicates the testset that is being controlled and the current switch state.
- Testset path switching occurs just before a channel is triggered. If a [channel trigger state is Hold](#), switching for that channel does not occur.
- PNA sweep speed will be slightly slower when using the E5091A to switch measurement paths.

### Connect and Configure the E5091A

The E5091A can be connected to any one of the PNA USB ports. When first installed, Windows will automatically launch the "Add New Hardware" wizard. Click **Next** to install the E5091A Testset.

---


**Note:** See the [power handling limitations](#) of the PNA USB ports.

---

Connect the PNA test ports to the E5091A test ports. Match PNA test port 1 to E5091A test port 1, and so forth.

### Selecting ID for E5091A


The PNA can control up to two E5091A testsets. Set the Instrument ID bit switch to 1 or 2. The testsets will then be identified automatically and referred to by the DIP switch setting on the E5091A rear-panel. Change the ID bit switch setting before connecting to the PNA USB.

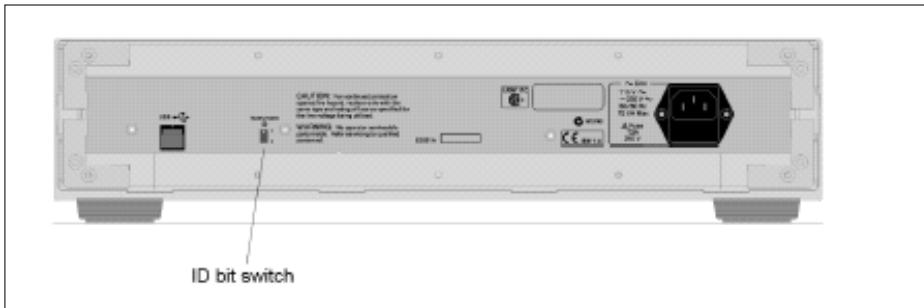


## Power ON

Immediately after power-on, all of the port connection indicator LEDs of the E5091A go ON. Then, after the PNA detects the E5091A, the four LEDs that indicate the connected test ports remain ON. If the PNA is not powered on or if the E5091A is not connected using a USB cable, all of the LEDs stay ON.

## How to make E5091A Testset Control Settings

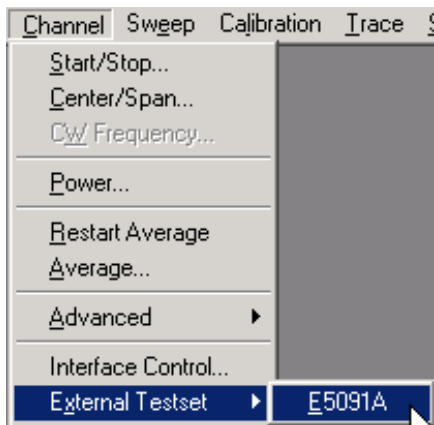

Learn more about using the [front panel interface](#)

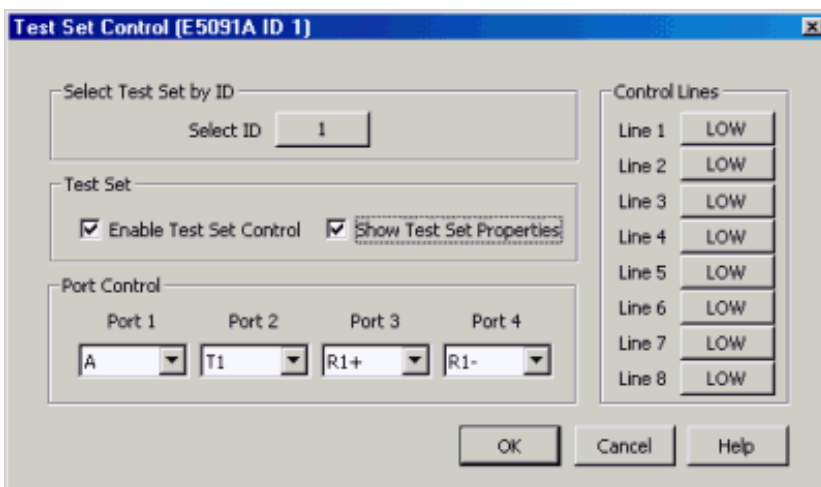


## E5091A Testset control dialog box help

The title of the dialog shows the test set model and ID number of the active testset..

**Select ID** ID of the testset to be configured. Up to two E5091A testsets can be controlled. Click to change testset ID. [Learn how to set the testset ID.](#)

**Enable Test Set Control** When cleared, port switching and control line settings are disabled. This selection affects all channels using the selected testset.

**Show Test Set Property** When checked, a second row on the status bar appears which indicates the testset that is being controlled and the current switch state. For example, the following image shows the status bar when two testsets are enabled using the above Port Control settings.



The "Interface control label" to the right of the red highlight is enabled using the [Interface Control](#) feature.

Learn more about the primary [status bar](#).

**Note:** The following two settings effect the channel of the active (selected) measurement. These settings will occur as the channel is being measured.

**Port Control** Switch paths through the test set. When first opened, the selections reflect the current switch settings. If no test set is found, default settings are displayed.

**Control Lines** Specifies the values of individual control lines. These general purpose control lines on the E5091A front-panel can be used in your test setup. Each button toggles the control line HIGH and LOW. When first opened, the selections reflect the current control lines. See your E5091A documentation for more information about the control lines.

**OK** When clicked, the changes to the dialog box are implemented and the port selections and control values are immediately sent to the specified test sets. The Port Control and Control line settings are stored with other channel data and used when those channels are swept.

**Cancel** (or Escape) Changes to the dialog are not implemented and revert to the settings before the dialog box was opened.

## Calibrating with the E5091A

The following are a few changes in the way you calibrate the PNA with the E5091A connected:

1. Create the measurements for the channel and configure the Port Control (switching) on the E5091A Testset Control dialog box. Enable **Show Testset Property**.
2. To calibrate, start the Calibration wizard and select a Calibration method (ECAL, SmartCal, Unguided).
3. Select the DUT connectors that are used at the E5091A measurement reference plane.
4. When prompted to connect a standard to a PNA port, instead connect the standard to the E5091A port as indicated on the Testset status bar. For example, if the status bar indicates **1 A**, instead of connecting a standard to port 1, connect it to port A reference plane of the E5091A.

# Technical Specifications for the E8356A, E8357A, E8358A

(Rev. 2004-04-23)

---

This is a complete list of the E8356A, E8357A, and E8358A network analyzer technical specifications.

- To optimize viewing of uncertainty curves, click the Maximize button.
- To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "E835xA Specifications"
- The uncertainty curves contained in this document apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the [equations](#) used to generate the uncertainty curves.

---

## **Definitions**

### **Corrected System Performance**

#### **System Dynamic Range**

#### **Type-N Connectors**

#### **3.5 mm Connectors**

#### **7-16 Connectors**

### **Uncorrected Instrument Performance**

#### **Test Port Output Characteristics (Source)**

#### **Test Port and Receiver Input Characteristics**

### **General Information**

#### **Front-panel Jumper Specs**

#### **Measurement Throughput Summary**

#### **Test Set Block Diagram**

#### **Test Set with Option 015 Block Diagram**

---

**See Specs for other PNA models**

## **Definitions**

All specifications and characteristics apply over a 25 °C ±5 °C range (unless otherwise stated) and 90 minutes after the instrument has been turned on.

**Specification (spec.):** Warranted performance. Specifications include guardbands to account for the expected

statistical performance distribution, measurement uncertainties, and changes in performance due to environmental conditions.

**Characteristic (char.):** A performance parameter that the product is expected to meet before it leaves the factory, but that is not verified in the field and is not covered by the product warranty. A characteristic includes the same guardbands as a specification.

**Typical (typ.):** Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Nominal (nom.):** A general, descriptive term that does not imply a level of performance. It is not covered by the product warranty.

**Calibration:** The process of measuring known standards to characterize a network analyzer's systematic (repeatable) errors.

**Corrected (residual):** Indicates performance after error correction (calibration). It is determined by the quality of calibration standards and how well "known" they are, plus system repeatability, stability, and noise.

**Uncorrected (raw):** Indicates instrument performance without error correction. The uncorrected performance affects the stability of a calibration.

**Standard:** When referring to the analyzer, this includes no options unless noted otherwise.

---

## Corrected System Performance

The specifications in this section apply for measurements made with the E8356A, E8357A, and E8358A analyzer with the following conditions:

- 10 Hz IF bandwidth
- No averaging applied to data
- Environmental temperature of 25 °C  $\pm$ 5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted

---

**Note:** The uncertainty curves contained in these specifications apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the equations used to generate the uncertainty curves.

---

### System Dynamic Range

#### Type-N Connectors

#### 3.5 mm Connectors

#### 7/16 Connectors

## Table 1. System Dynamic Range



| Description                                              | Specification (dB) | Characteristic (dB) |
|----------------------------------------------------------|--------------------|---------------------|
| <b>Dynamic range<sup>a</sup><br/>(at test port)</b>      |                    |                     |
| 300 kHz to 25 MHz <sup>b</sup>                           | 125                |                     |
| 25 MHz to 3 GHz <sup>b</sup>                             | 128                |                     |
| 3 GHz to 6 GHz                                           | 118                |                     |
| 6 GHz to 9 GHz                                           | 113                |                     |
| <b>Dynamic range<sup>c</sup><br/>(at receiver input)</b> |                    |                     |
| 300 kHz to 25 MHz <sup>d</sup>                           |                    | 140                 |
| 25 MHz to 3 GHz <sup>d</sup>                             |                    | 143                 |
| 3 GHz to 6 GHz                                           |                    | 133                 |
| 6 GHz to 9 GHz                                           |                    | 128                 |

**a** The test port dynamic range is calculated as the difference between the test port rms noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account.

**b** May be limited to 100 dB at particular frequencies below 750 MHz due to spurious receiver residuals.

**c** The receiver input dynamic range is calculated as the difference between the receiver rms noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its damage level. When the analyzer is in segment sweep mode, frequency segments can be defined with a higher power level when the extended dynamic range is required (i.e. the portion of the device's response with high insertion loss), and reduced power when receiver damage may occur (i.e. the portion of the device's response with low insertion loss).

**d** May be limited to 115 dB at particular frequencies below 750 MHz due to spurious receiver residuals.

**Note:** Receiver Dynamic Range specifications are not included in this E8356/7/8A document.

## Corrected System Performance with Type-N Connectors

### 85032F Calibration Kit

### 85092C Electronic Calibration Module

---

**Note:** This document provides technical specifications for the following calibration kits only: 85032F, 85092C, 85033E, 85093C and 85038A.

---



## Table 2. Corrected System Performance With Type-N Device Connectors, 85032F Calibration Kit

Applies to the E8356A, E8357A, and E8358A analyzer, 85032F (Type-N, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:



- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted

| Description           | Specification (dB) |                  |             |             |
|-----------------------|--------------------|------------------|-------------|-------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz  | 6 to 9 GHz  |
| Directivity           | 49                 | 46               | 40          | 38          |
| Source Match          | 41                 | 40               | 36          | 35          |
| Load Match            | 49                 | 45               | 39          | 37          |
| Reflection Tracking   | $\pm 0.011$        | $\pm 0.021$      | $\pm 0.032$ | $\pm 0.054$ |
| Transmission Tracking | $\pm 0.011$        | $\pm 0.019$      | $\pm 0.041$ | $\pm 0.051$ |

**Transmission Uncertainty (Specifications)**

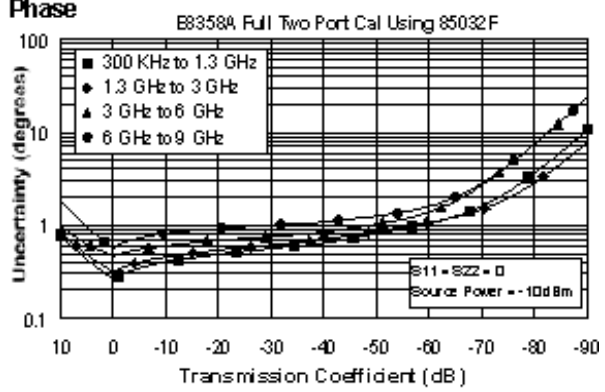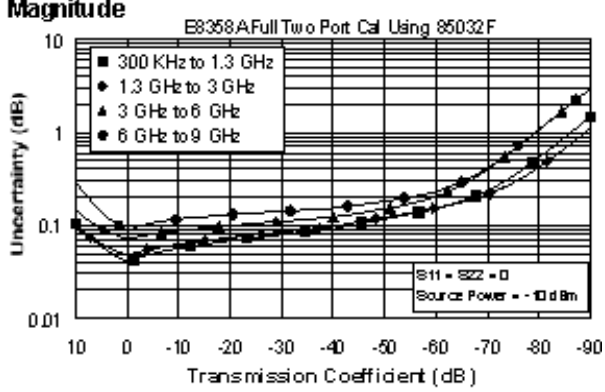

**Reflection Uncertainty (Specifications)**

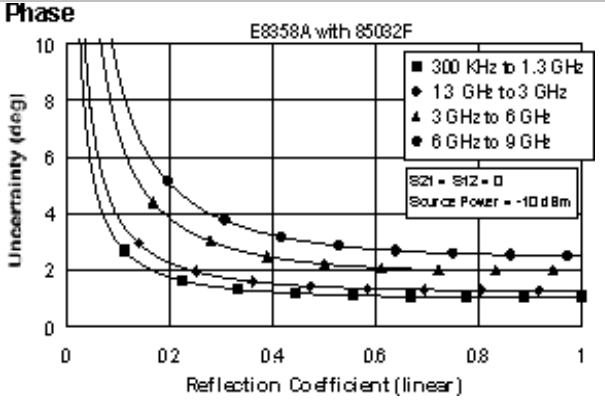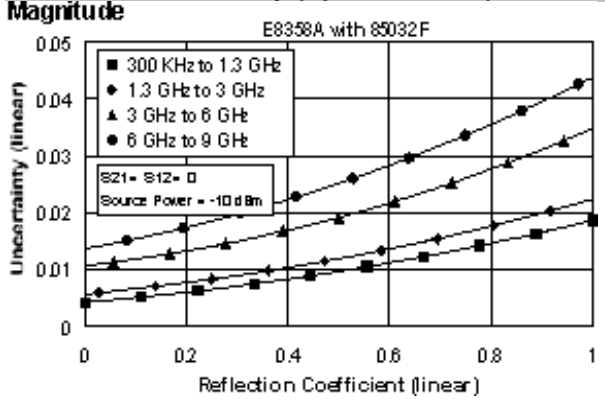

**Table 3. Corrected System Performance With Type-N Device Connectors, Option 015 With 85032F Calibration Kit**


Applies to the E8356A, E8357A, and E8358A analyzer with Option 015, 85032F (Type-N, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |             |             |
|-----------------------|--------------------|------------------|-------------|-------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz  | 6 to 9 GHz  |
| Directivity           | 49                 | 46               | 40          | 38          |
| Source Match          | 41                 | 40               | 36          | 35          |
| Load Match            | 49                 | 45               | 39          | 37          |
| Reflection Tracking   | $\pm 0.011$        | $\pm 0.021$      | $\pm 0.032$ | $\pm 0.054$ |
| Transmission Tracking | $\pm 0.011$        | $\pm 0.024$      | $\pm 0.052$ | $\pm 0.065$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

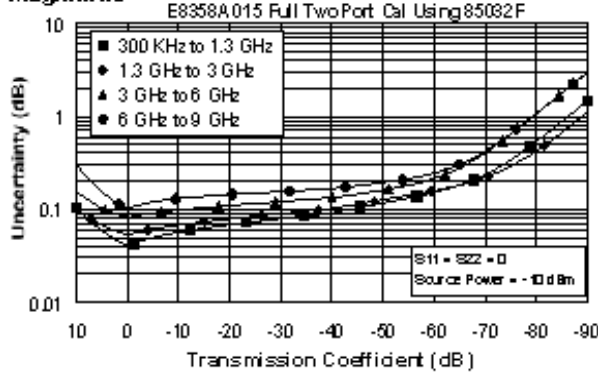


#### Phase

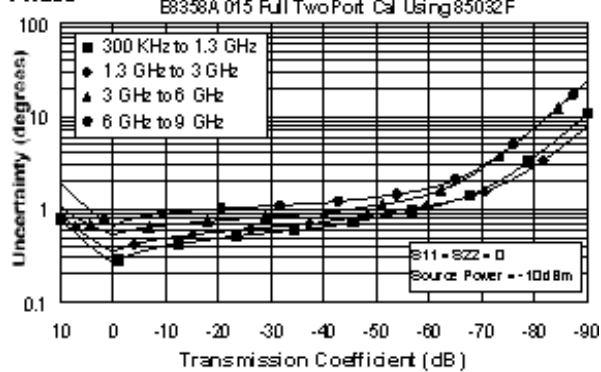


### Reflection Uncertainty (Specifications)

#### Magnitude

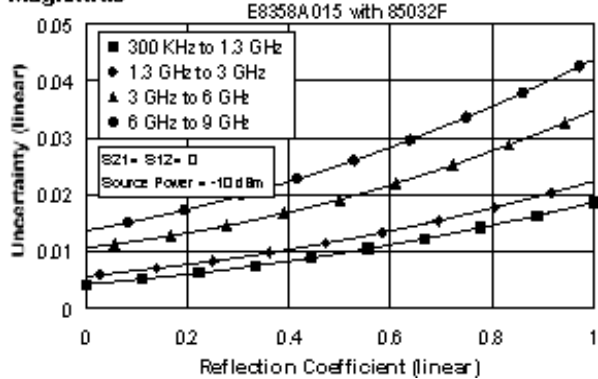

#### Phase

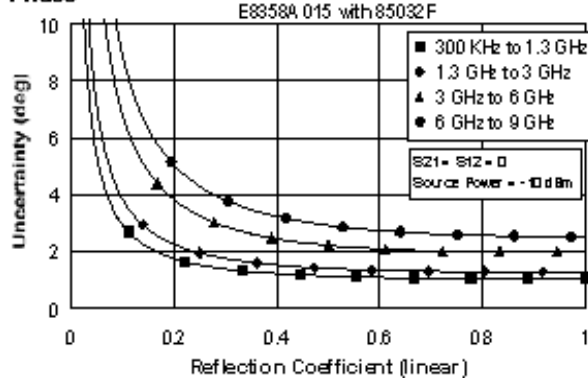



**Table 4. Corrected System Performance With Type-N Device Connectors, 85092C Electronic Calibration Module**

Applies to the E8356A, E8357A, and E8358A analyzer, 85092C (Type-N, 50Ω) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:



- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted

| Description           | Specification (dB) |                  |           |                         |
|-----------------------|--------------------|------------------|-----------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 Hz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 54               | 52        | 47                      |
| Source Match          | 45                 | 44               | 41        | 36                      |
| Load Match            | 47                 | 47               | 44        | 39                      |
| Reflection Tracking   | ±0.040             | ±0.040           | ±0.060    | ±0.070                  |
| Transmission Tracking | ±0.039             | ±0.039           | ±0.068    | ±0.135                  |

**Transmission Uncertainty (Specifications)**

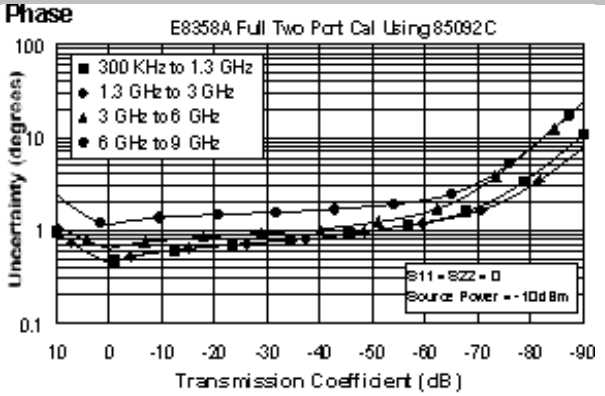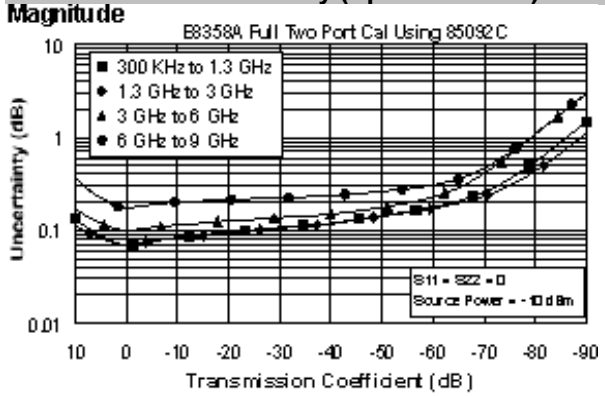

**Reflection Uncertainty (Specifications)**

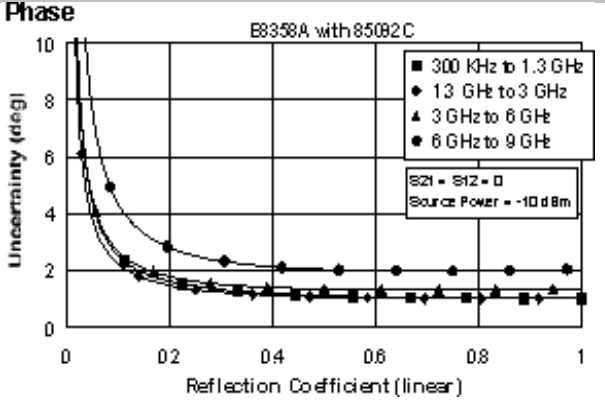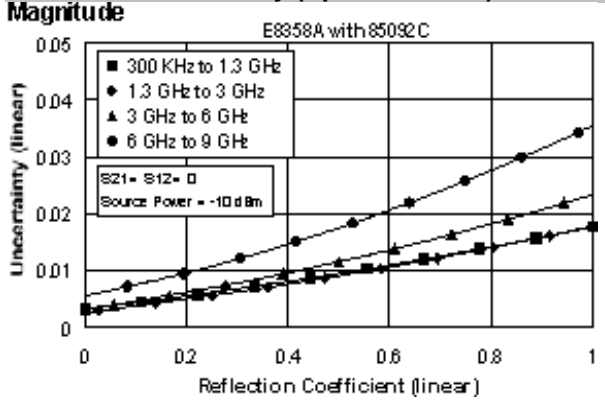

**Table 5. Corrected System Performance With Type-N Device Connectors, Option 015 With 85092C Electronic Calibration Module**


Applies to the E8356A, E8357A, and E8358A analyzer with Option 015, 85092C (Type-N, 50Ω) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 54               | 52         | 47                      |
| Source Match          | 45                 | 44               | 41         | 36                      |
| Load Match            | 47                 | 47               | 44         | 39                      |
| Reflection Tracking   | ±0.040             | ±0.040           | ±0.060     | ±0.070                  |
| Transmission Tracking | ±0.039             | ±0.039           | ±0.068     | ±0.135                  |

**Transmission Uncertainty (Specifications)**

**Magnitude**

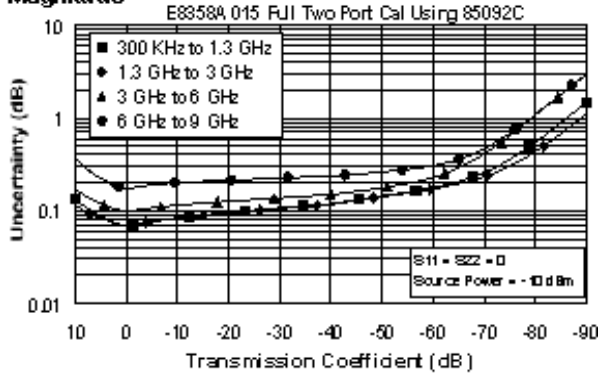


**Phase**

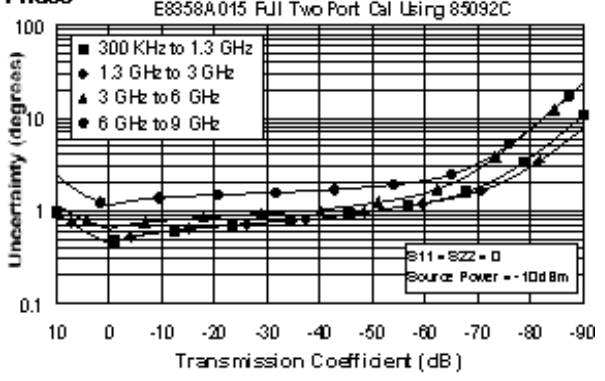


**Reflection Uncertainty (Specifications)**

**Magnitude**

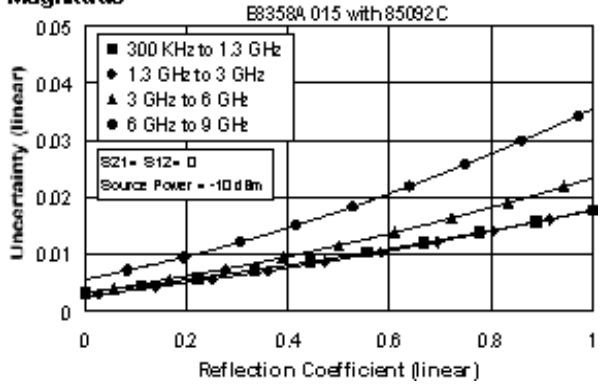

**Phase**

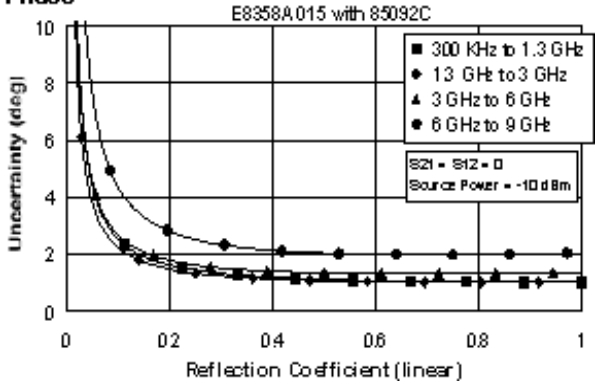

**Corrected System Performance with 3.5 mm Connectors**

[85033E Calibration Kit](#)

[Option 015 with 85033E Calibration Kit](#)

[85093C Electronic Calibration Module](#)

**Option 015 with 85093C Electronic Calibration Module**


**Table 6. Corrected System Performance With 3.5 mm Device Connector Type, 85033E Calibration Kit**

Applies to the E8356A, E8357A, and E8358A analyzer, 85033E (3.5 mm, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:


- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted

| Description           | Specification (dB) |                  |            |            |
|-----------------------|--------------------|------------------|------------|------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz |
| Directivity           | 46                 | 44               | 38         | 38         |
| Source Match          | 43                 | 40               | 37         | 36         |
| Load Match            | 46                 | 44               | 38         | 38         |
| Reflection Tracking   | ±0.006             | ±0.007           | ±0.009     | ±0.010     |
| Transmission Tracking | ±0.011             | ±0.020           | ±0.041     | ±0.047     |

**Transmission Uncertainty (Specifications)**  
**Magnitude**

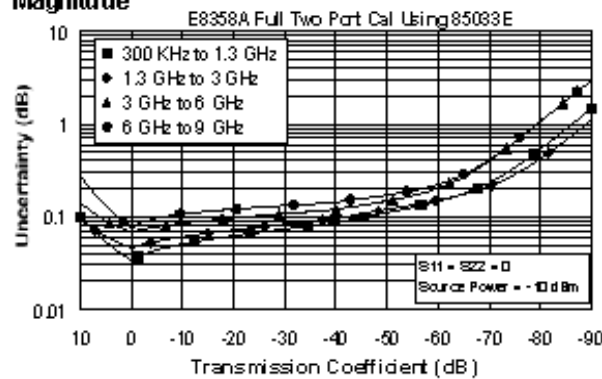


**Phase**

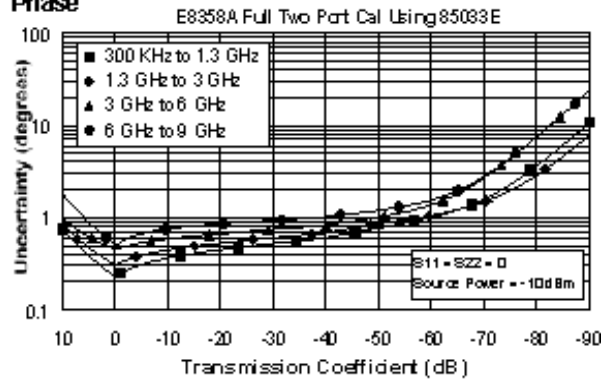


**Reflection Uncertainty (Specifications)**

**Magnitude**

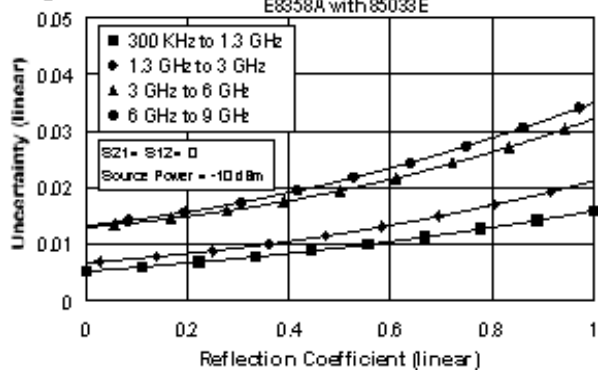

**Phase**

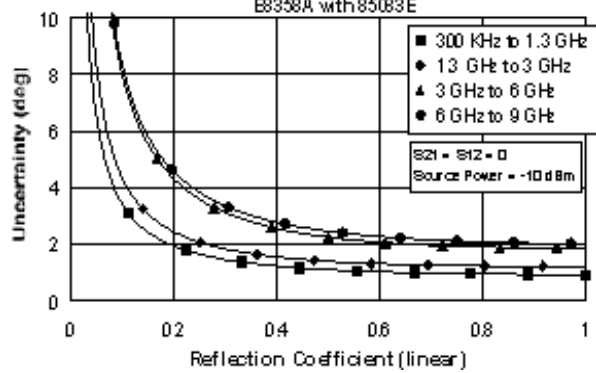

**Table 7. Corrected System Performance With 3.5 mm Device Connector Type, Option 015 With 85033E Calibration Kit**


Applies to the E8356A, E8357A, and E8358A analyzer with Option 015, 85033E (3.5 mm, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |            |
|-----------------------|--------------------|------------------|------------|------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz |
| Directivity           | 46                 | 44               | 38         | 38         |
| Source Match          | 43                 | 40               | 37         | 36         |
| Load Match            | 46                 | 44               | 38         | 38         |
| Reflection Tracking   | ±0.006             | ±0.007           | ±0.009     | ±0.010     |
| Transmission Tracking | ±0.011             | ±0.025           | ±0.052     | ±0.059     |

**Transmission Uncertainty (Specifications)**

**Magnitude**

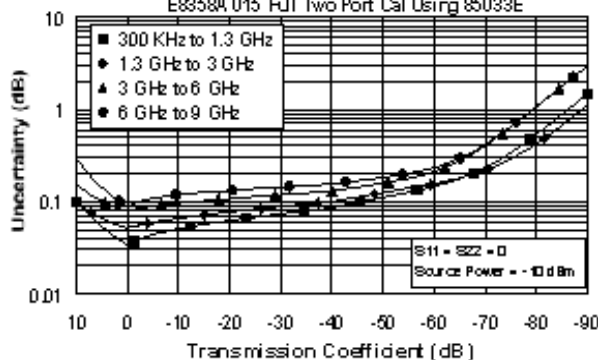


**Phase**

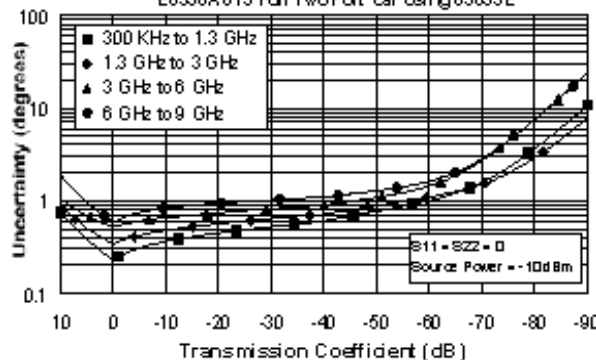


## Reflection Uncertainty (Specifications)

### Magnitude

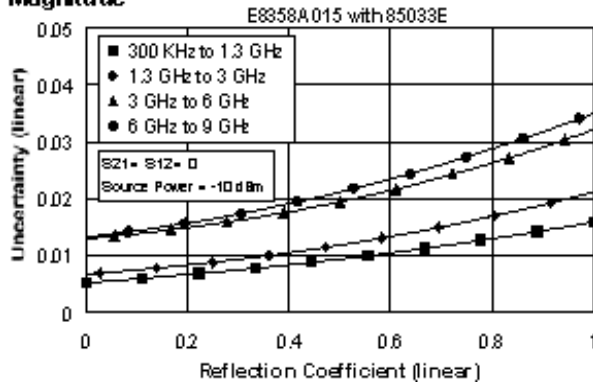

### Phase

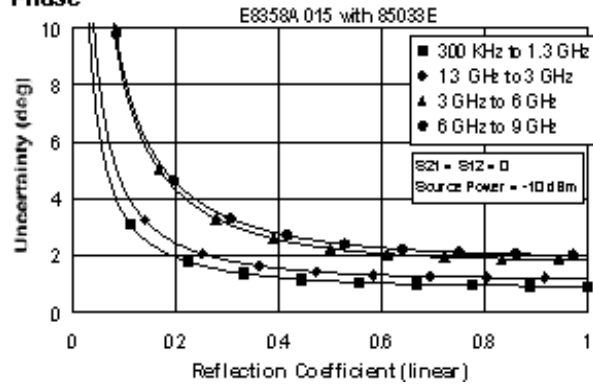

**Table 8. Corrected System Performance With 3.5 mm Device Connector Type, 85093C Electronic Calibration Module**


Applies to the E8356A, E8357A, and E8358A analyzer, 85093C (3.5 mm, 50 $\Omega$ ) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25°  $\pm$ 5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |             |                         |
|-----------------------|--------------------|------------------|-------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz  | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 52               | 51          | 47                      |
| Source Match          | 44                 | 44               | 39          | 34                      |
| Load Match            | 47                 | 47               | 44          | 40                      |
| Reflection Tracking   | $\pm 0.030$        | $\pm 0.040$      | $\pm 0.050$ | $\pm 0.070$             |
| Transmission Tracking | $\pm 0.039$        | $\pm 0.049$      | $\pm 0.068$ | $\pm 0.116$             |

## Transmission Uncertainty (Specifications)

### Magnitude

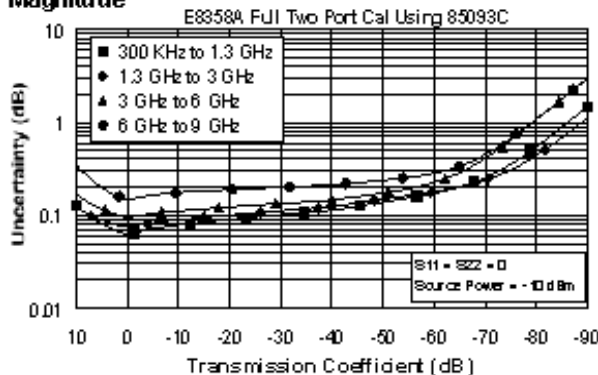


### Phase

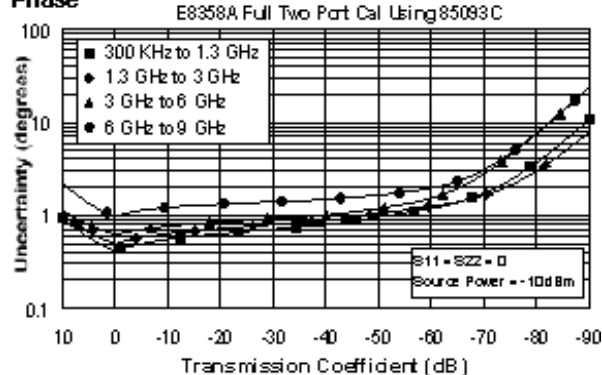




## Reflection Uncertainty (Specifications)

### Magnitude

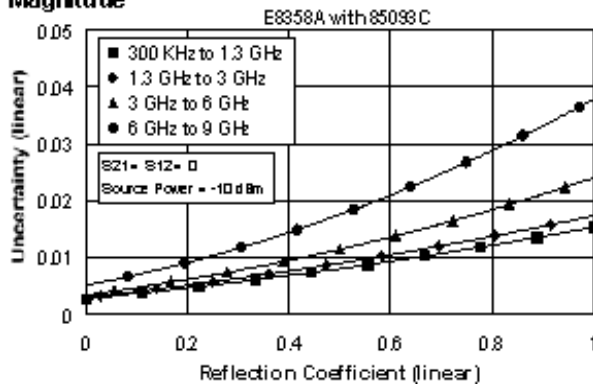

### Phase

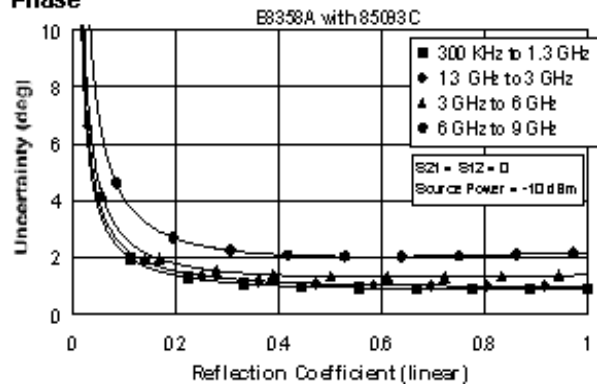

**Table 9. Corrected System Performance With 3.5 mm Device Connector Type, Option 015 With 85093C Electronic Calibration Module**


Applies to the E8356A, E8357A, and E8358A analyzer with Option 015, 85093C (3.5 mm, 50Ω) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 52               | 51         | 47                      |
| Source Match          | 44                 | 44               | 39         | 34                      |
| Load Match            | 47                 | 47               | 44         | 40                      |
| Reflection Tracking   | ±0.030             | ±0.040           | ±0.050     | ±0.070                  |
| Transmission Tracking | ±0.039             | ±0.049           | ±0.068     | ±0.116                  |

## Transmission Uncertainty (Specifications)

### Magnitude

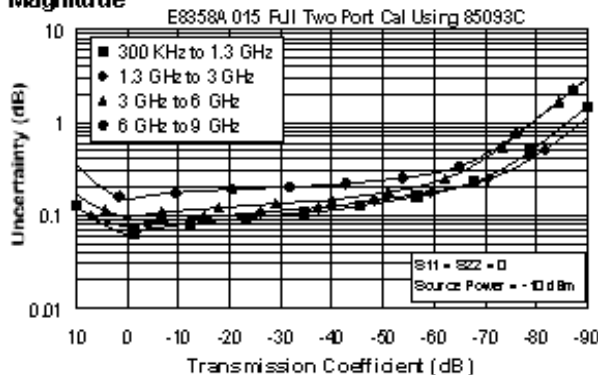


### Phase

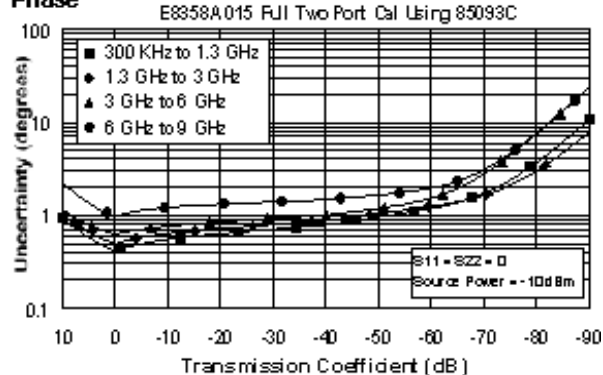


## Reflection Uncertainty (Specifications)

### Magnitude

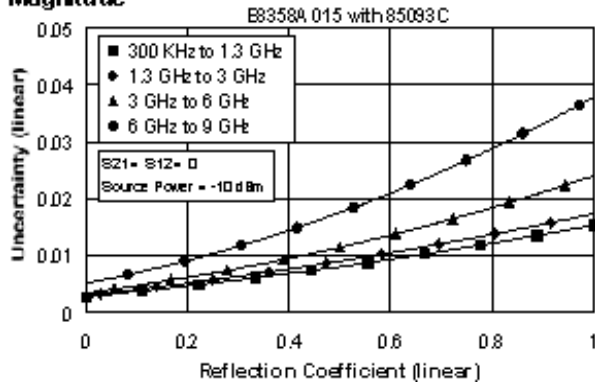

### Phase

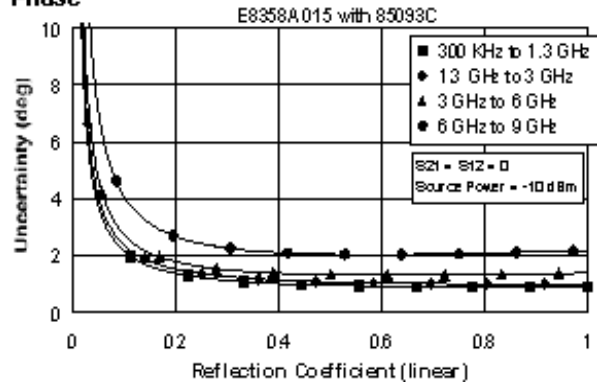

## Corrected System Performance with 7-16 Connectors

### 85038A Calibration Kit

### Option 015 with 85038A Calibration Kit

**Table 10. Corrected System Performance With 7-16 Device Connector Type, 85038A Calibration Kit**


Applies to the E8356A, E8357A, and E8358A analyzer, 85038A (7-16, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 40                 | 40               | 36         | 36                      |
| Source Match          | 37                 | 37               | 34         | 34                      |
| Load Match            | 39                 | 39               | 35         | 35                      |
| Reflection Tracking   | ±0.089             | ±0.089           | ±0.115     | ±0.115                  |
| Transmission Tracking | ±0.022             | ±0.031           | ±0.059     | ±0.062                  |

## Transmission Uncertainty (Specifications)

### Magnitude

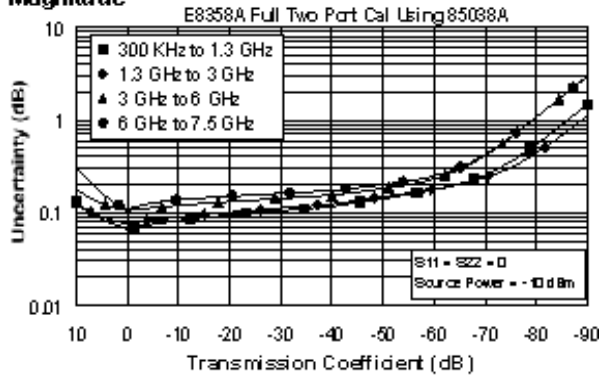


### Phase

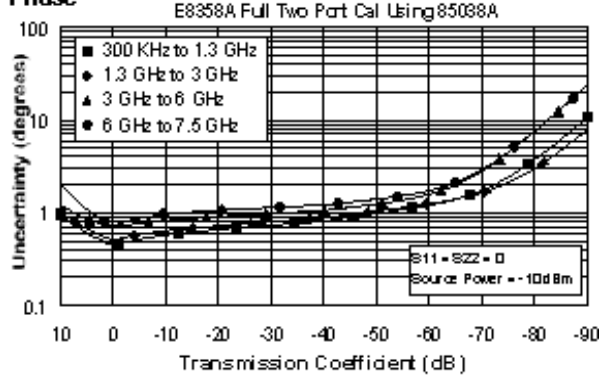


### Reflection Uncertainty (Specifications)

#### Magnitude

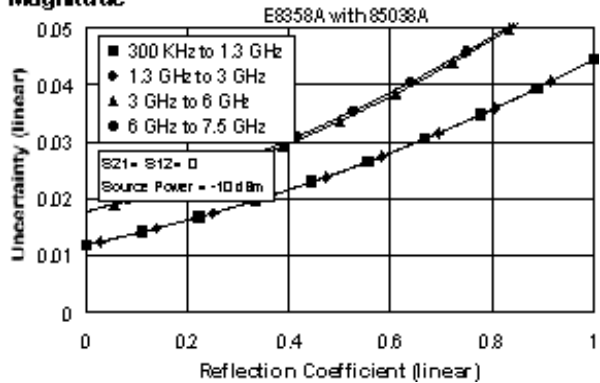

#### Phase

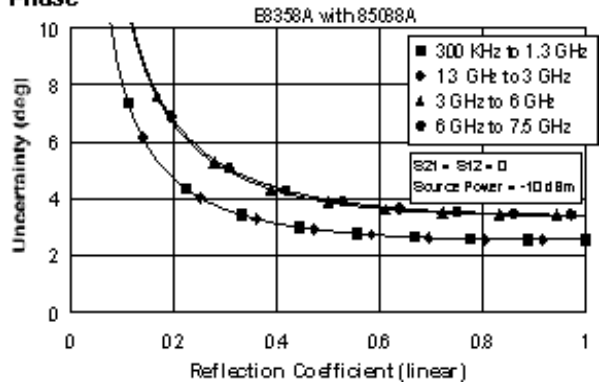

**Table 11. Corrected System Performance With 7-16 Device Connector Type, Option 015 With 85038A Calibration Kit**


Applies to the E8356A, E8357A, and E8358A analyzer with Option 015, 85038A (7-16, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 40                 | 40               | 36         | 36                      |
| Source Match          | 37                 | 37               | 34         | 34                      |
| Load Match            | 39                 | 39               | 35         | 35                      |
| Reflection Tracking   | ±0.089             | ±0.089           | ±0.115     | ±0.115                  |
| Transmission Tracking | ±0.022             | ±0.040           | ±0.075     | ±0.080                  |

### Transmission Uncertainty (Specifications)

### Magnitude

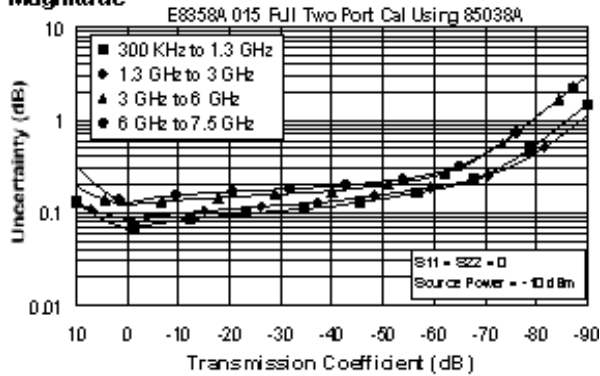


### Phase

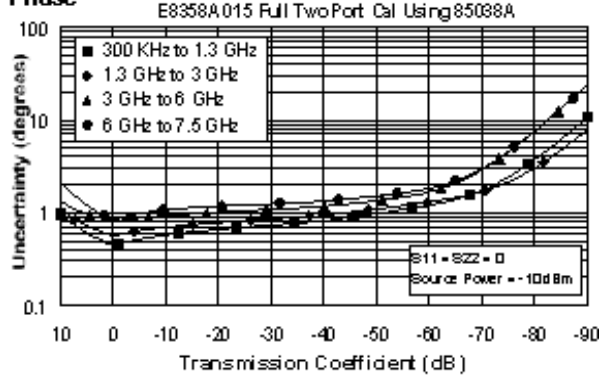


### Reflection Uncertainty (Specifications)

#### Magnitude

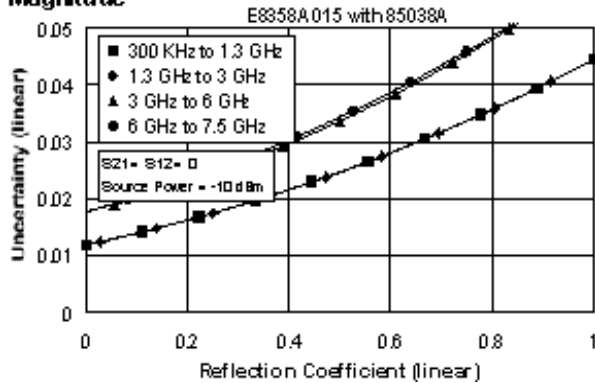

#### Phase

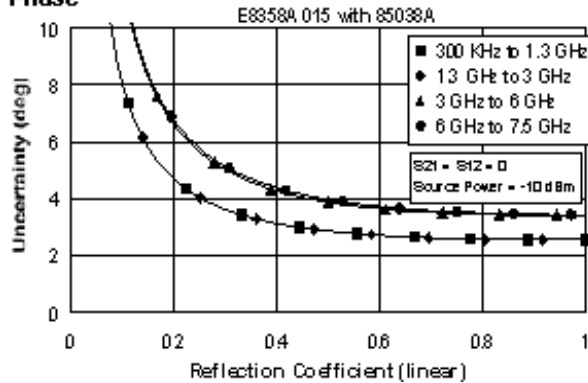

### Uncorrected Instrument Performance

Table 12. Uncorrected Instrument Performance

| Description             | Specification (dB) |                 |                  |                |                |
|-------------------------|--------------------|-----------------|------------------|----------------|----------------|
|                         | 300 kHz to 1 MHz   | 1MHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 GHz to 6 GHz | 6 GHz to 9 GHz |
| Directivity             | 30                 | 33              | 27               | 20             | 13             |
| Source Match            | 20                 | 20              | 17               | 15             | 14             |
| Source Match (Opt. 015) | 20                 | 20              | 15               | 13             | 12             |
| Load Match              | 20                 | 20              | 17               | 15             | 15             |
| Load Match (Opt. 015)   | 20                 | 20              | 15               | 13             | 13             |
| Reflection Tracking     | ±1.5               | ±1.5            | ±1.5             | ±2.5           | ±3.0           |
| Transmission Tracking   | ±1.5               | ±1.5            | ±1.5             | ±2.5           | ±3.0           |

### Test Port Output Characteristics (Source)

#### Output Frequency

## Output Power

## Output Signal Purity

**Table 13. Test Port Output Frequency**

| Description             | Specification      | Supplemental Information                                   |
|-------------------------|--------------------|------------------------------------------------------------|
| <b>Range</b>            |                    |                                                            |
| E8356A                  | 300 kHz to 3.0 GHz |                                                            |
| E8357A                  | 300 kHz to 6.0 GHz |                                                            |
| E8358A                  | 300 kHz to 9.0 GHz |                                                            |
| <b>Resolution</b>       | 1 Hz               |                                                            |
| <b>Source Stability</b> |                    | ±0.05 ppm, -0° to 40 °C, typical<br>±0.1 ppm/year, typical |
| <b>CW Accuracy</b>      | ±1 ppm             |                                                            |

**Table 14. Test Port Output Power<sup>a</sup>**

| Description              | Specification  | Supplemental Information                                                            |
|--------------------------|----------------|-------------------------------------------------------------------------------------|
| <b>Level Accuracy</b>    |                |                                                                                     |
|                          |                | Variation from 0 dBm in power range 0 (step attenuator at 0 dB) ±1.5dB below 10 MHz |
| 300 kHz to 10 MHz        | ±1.5 dB        |                                                                                     |
| 10 MHz to 6 GHz          | ±1.0 dB        |                                                                                     |
| 6 GHz to 9 GHz           | ±2.0 dB        |                                                                                     |
| <b>Level Linearity</b>   |                |                                                                                     |
|                          |                | Variation from 0 dBm in power range 0                                               |
| 300 kHz to 9 GHz         | ±0.3 dB        | -15 to +5 dBm                                                                       |
| 300 kHz to 1 MHz         | ±1.0 dB        | +5 to +10 dBm                                                                       |
| 1 MHz to 6 GHz           | ±0.5 dB        | +5 to +10 dBm                                                                       |
| <b>Range<sup>b</sup></b> |                |                                                                                     |
| 300 kHz to 6 GHz         | -85 to +10 dBm |                                                                                     |
| 6 GHz to 9 GHz           | -85 to +5 dBm  |                                                                                     |

| Sweep Range             |         |  |
|-------------------------|---------|--|
| 300 kHz to 6 GHz        | 25 dB   |  |
| 6 GHz to 9 GHz          | 20 dB   |  |
| <b>Level Resolution</b> | 0.01 dB |  |

**a** Source output performance on port 1 only. Port 2 output performance is typical.

**b** Power to which the source can be set and phase lock is assured.

**Table 15. Test Port Output Signal Purity**

| Description                           | Specification | Supplemental Information                                       |
|---------------------------------------|---------------|----------------------------------------------------------------|
| <b>Harmonics (2nd or 3rd)</b>         |               |                                                                |
| at max output power (< 25 MHz)        |               | < -25 dBc, typical                                             |
| at max output power (25 MHz to 9 GHz) |               | < -25 dBc, characteristic <sup>a</sup>                         |
| at 0 dBm output                       |               | < -35 dBc, typical                                             |
| at -10 dBm output                     |               | < -38 dBc, typical, in power range 0 (step attenuator at 0 dB) |
| <b>Non-harmonic Spurious</b>          |               |                                                                |
| at max output                         |               | -30 dBc, typical for offset freq >1kHz                         |
| at -10 dBm output                     |               | -50 dBc, typical for offset freq >1kHz                         |

**a** Typical below 25 MHz.

## Test Port and Receiver Input Characteristics

### Input Levels

### Trace Noise

### Reference Level and Stability

### Dynamic Accuracy

### Group Delay

**Table 16. Test Port and Receiver Input Levels**

| Description                          | Specification | Supplemental Information |
|--------------------------------------|---------------|--------------------------|
| <b>Maximum Test Port Input Level</b> |               |                          |
| <b>Test Ports 1 and 2:</b>           |               |                          |
| 300 kHz to 25 MHz                    | +10 dBm       | < 0.6 dB compression     |

|                                          |                 |                               |
|------------------------------------------|-----------------|-------------------------------|
| 25 MHz to 3 GHz                          | +10 dBm         | < 0.4 dB compression          |
| 3 GHz to 6 GHz                           | +10 dBm         | < 0.7 dB compression          |
| 6 GHz to 9 GHz                           | +5 dBm          | < 0.7 dB compression          |
| <b>Damage Level</b>                      |                 |                               |
| Test Port 1, 2                           |                 | +30 dBm or $\pm 30$ VDC, typ. |
| R1, R2 IN                                |                 | +15 dBm or $\pm 5$ VDC, typ.  |
| A, B IN (standard)                       |                 | +15 dBm or $\pm 5$ VDC, typ.  |
| A, B IN (Opt. 015)                       |                 | +15 dBm or $\pm 0$ VDC, typ.  |
| Coupler IN (Opt. 015)                    |                 | +33 dBm or $\pm 0$ VDC, typ.  |
| <b>Test Port Noise Floor<sup>a</sup></b> |                 |                               |
| 300 kHz to 25 MHz <sup>b</sup>           |                 |                               |
| 10 Hz IF Bandwidth                       | = -115 dBm      |                               |
| 1 kHz IF Bandwidth                       | = -95 dBm       |                               |
| 25 MHz to 3 GHz <sup>b</sup>             |                 |                               |
| 10 Hz IF Bandwidth                       | = -118 dBm      |                               |
| 1 kHz IF Bandwidth                       | = -98 dBm       |                               |
| 3 GHz to 9 GHz                           |                 |                               |
| 10 Hz IF Bandwidth                       | $\leq$ -108 dBm |                               |
| 1 kHz IF Bandwidth                       | $\leq$ -88 dBm  |                               |
| <b>Receiver Noise Floor<sup>a</sup></b>  |                 |                               |
| 300 kHz to 25 MHz <sup>c</sup>           |                 |                               |
| 10 Hz IF Bandwidth                       | $\leq$ -130 dBm |                               |
| 1 kHz IF Bandwidth                       | $\leq$ -110 dBm |                               |
| 25 MHz to 3 GHz <sup>c</sup>             |                 |                               |
| 10 Hz IF Bandwidth                       | $\leq$ -133 dBm |                               |
| 1 kHz IF Bandwidth                       | $\leq$ -113 dBm |                               |
| 6 GHz to 9 GHz                           |                 |                               |
| 10 Hz IF Bandwidth                       | $\leq$ -123 dBm |                               |

|                                                    |                 |                                                               |
|----------------------------------------------------|-----------------|---------------------------------------------------------------|
| 1 kHz IF Bandwidth                                 | $\leq -103$ dBm |                                                               |
| <b>Crosstalk</b>                                   |                 |                                                               |
|                                                    |                 | Between test ports 1 and 2, with short circuits at both ports |
| 300 kHz to 1 MHz                                   | $< -120$ dB     |                                                               |
| 1 MHz to 25 MHz                                    | $< -125$ dB     |                                                               |
| 25 MHz to 3 GHz                                    | $< -128$ dB     |                                                               |
| 3 GHz to 6 GHz                                     | $< -118$ dB     |                                                               |
| 6 GHz to 9 GHz                                     | $< -113$ dB     |                                                               |
| <b>Maximum Receiver Input Level (A, B, R1, R2)</b> |                 |                                                               |
| 300 kHz to 6 GHz                                   |                 | -6 dBm, typical                                               |
| 6 GHz to 9 GHz                                     |                 | -11 dBm, typical                                              |
| <b>Reference Input Level (R1, R2)<sup>d</sup></b>  |                 |                                                               |
| 300 kHz to 9 GHz                                   |                 | -10 to -35 dBm, typical                                       |
| <b>Maximum Coupler Input Level (Opt 015)</b>       |                 |                                                               |
| 300 kHz to 9 GHz                                   |                 | +33 dBm, typical                                              |

<sup>a</sup> Total average (RMS) noise power calculated as the mean value of a linear magnitude trace expressed in dBm.

<sup>b</sup> May be limited to -90 dBm at particular frequencies below 750 MHz due to spurious receiver residuals.

<sup>c</sup> May be limited to -105 dBm at particular frequencies below 750 MHz due to spurious receiver residuals.

<sup>d</sup> Input level to maintain phase lock.

**Table 17. Test Port Input (Trace Noise)**

| Description                              | Specification       | Supplemental Information |
|------------------------------------------|---------------------|--------------------------|
| <b>Trace Noise<sup>a</sup> Magnitude</b> |                     |                          |
| 1 kHz IF Bandwidth                       | $< 0.002$ dB rms    |                          |
| 10 kHz IF Bandwidth                      | $< 0.005$ dB rms    |                          |
| <b>Trace Noise<sup>a</sup> Phase</b>     |                     |                          |
| 1 kHz IF Bandwidth                       | $< 0.010^\circ$ rms |                          |
| 10 kHz IF Bandwidth                      | $< 0.035^\circ$ rms |                          |

<sup>a</sup> Trace noise is defined as a ratio measurement of a through or a full reflection, with the source set to 0 dBm.

**Table 18. Test Port Input (Reference Level and Stability)**



| Description                            | Specification | Supplemental Information |
|----------------------------------------|---------------|--------------------------|
| <b>Reference Level Magnitude</b>       |               |                          |
| Range                                  | ±200 dB       |                          |
| Resolution                             | 0.001 dB      |                          |
| <b>Reference Level Phase</b>           |               |                          |
| Range                                  | ±500°         |                          |
| Resolution                             | 0.01°         |                          |
| <b>Stability Magnitude<sup>a</sup></b> |               |                          |
| 300 kHz to 3 GHz                       |               | 0.02 dB/°C, typical      |
| 3 GHz to 6 GHz                         |               | 0.04 dB/°C, typical      |
| 6 GHz to 9 GHz                         |               | 0.06 dB/°C, typical      |
| <b>Stability Phase<sup>a</sup></b>     |               |                          |
| 300 kHz to 3 GHz                       |               | 0.2°/°C, typical         |
| 3 GHz to 6 GHz                         |               | 0.3°/°C, typical         |
| 6 GHz to 9 GHz                         |               | 0.6°/°C, typical         |

<sup>a</sup> Stability is defined as a ratio measurement at the test port.



**Table 19. Test Port Input (Dynamic Accuracy specification<sup>a</sup>)**

Accuracy of the test port input power reading is relative to the reference input power level. Applies to input ports 1 and 2 with the following conditions:

- IF bandwidth = 10 Hz
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature



300 kHz to 3 GHz

300 kHz to 3 GHz

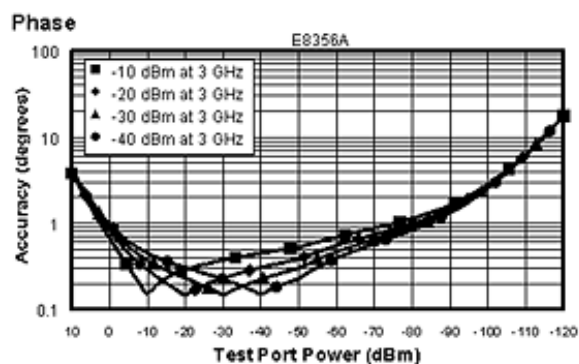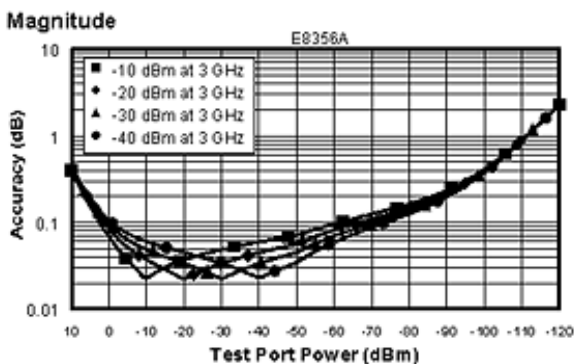



300 kHz to 6 GHz

300 kHz to 6 GHz

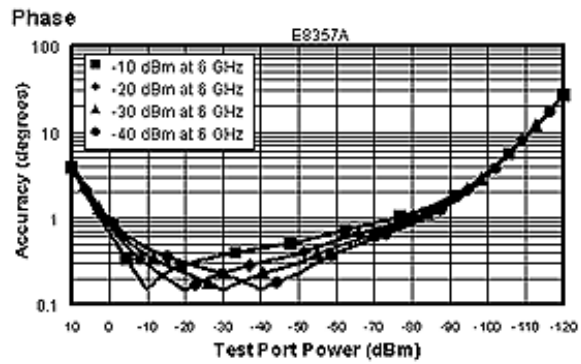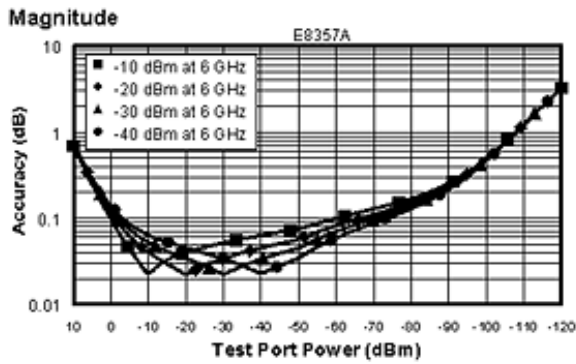

300 kHz to 9 GHz

300 kHz to 9 GHz

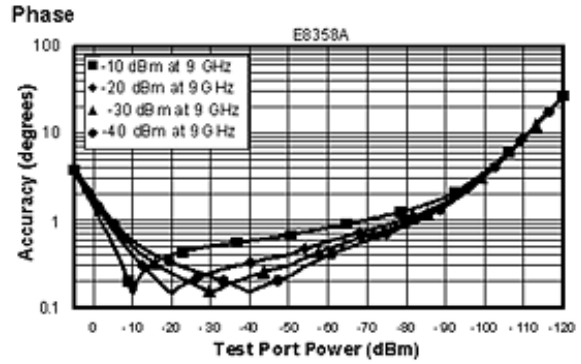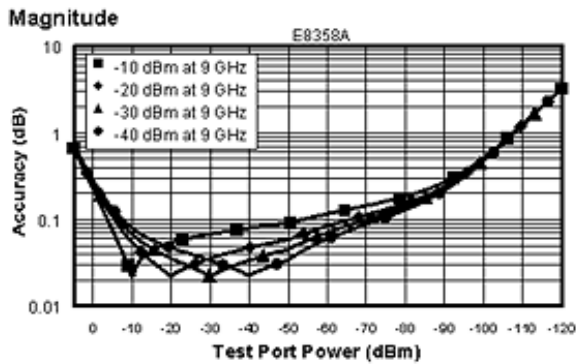


a Dynamic accuracy is verified with the following measurements:

- compression over frequency
- IF linearity at a single frequency of 1.195 GHz and a reference level of -20 dBm

**Table 20. Test Port Input (Group Delay)<sup>a</sup>**

| Description           | Specification                                           | Supplemental Information                                                             |
|-----------------------|---------------------------------------------------------|--------------------------------------------------------------------------------------|
| Aperture (selectable) | $(\text{frequency span})/(\text{number of points} - 1)$ |                                                                                      |
| Maximum Aperture      | 20% of frequency span                                   |                                                                                      |
| Range                 | $0.5 \times (1/\text{minimum aperture})$                |                                                                                      |
| Maximum Delay         |                                                         | Limited to measuring no more than 180° of phase change within the minimum aperture.) |
| Accuracy              |                                                         | See graph below. Char.                                                               |

The following graph shows group delay accuracy with type-N full 2-port calibration and a 10 Hz IF bandwidth. Insertion loss is assumed to be < 2 dB and electrical length to be ten meters.

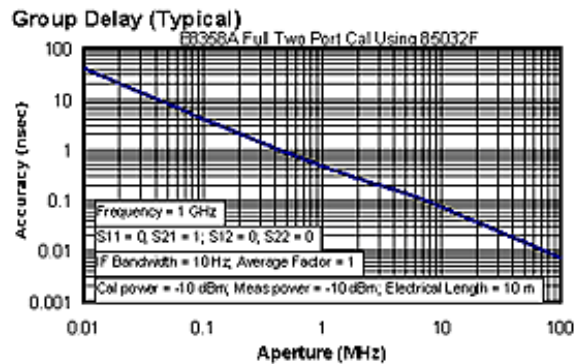

In general, the following formula can be used to determine the accuracy, in seconds, of specific group delay measurement:

$$\pm \text{Phase Accuracy (deg)} / [360 \times \text{Aperture (Hz)}]$$

Depending on the aperture and device length, the phase accuracy used is either incremental phase accuracy or worst case phase accuracy.

a Group delay is computed by measuring the phase change within a specified frequency step (determined by the frequency span and the number of points per sweep).

## General Information

### System Bandwidths

#### Front Panel

#### Rear Panel

### Environment and Dimensions

**Table 21. System Bandwidths**

| Description                  | Specification | Supplemental Information                                                                  |
|------------------------------|---------------|-------------------------------------------------------------------------------------------|
| <b>IF Bandwidth Settings</b> |               |                                                                                           |
| Range                        |               | 1 Hz to 40 kHz<br>in a 1, 2, 3, 5, 7, 10 sequence up to 30 kHz,<br>35 kHz, 40kHz, nominal |

**Table 22. Front Panel Information**

| Description               | Supplemental Information                                                                        |
|---------------------------|-------------------------------------------------------------------------------------------------|
| <b>RF Connectors</b>      |                                                                                                 |
| Type                      | Type-N, female; 50 $\Omega$ , nominal                                                           |
| Center Pin Protrusion     | 0.204 to 0.207 in., characteristic                                                              |
| <b>Probe Power</b>        |                                                                                                 |
| Connector                 | 3-pin connector, male                                                                           |
| Positive Supply           | +15 VDC $\pm$ 2%, 400 mA, max, characteristic                                                   |
| Negative Supply           | -12.6 VDC $\pm$ 5%, 300 mA, max, characteristic                                                 |
| <b>Display</b>            |                                                                                                 |
| Size                      | 21.3 cm (8.4 in) diagonal color active matrix LCD; 640 (horizontal) X 480 (vertical) resolution |
| Refresh Rate              | Vertical 59.83 Hz; Horizontal 31.41 Hz                                                          |
| <b>Display Range</b>      |                                                                                                 |
| Magnitude                 | $\pm$ 200 dB (at 20 dB/div), max                                                                |
| Phase                     | $\pm$ 180°, max                                                                                 |
| Polar                     | 10 pUnits, min<br>1000 Units, max                                                               |
| <b>Display Resolution</b> |                                                                                                 |
| Magnitude                 | 0.001 dB/div, min                                                                               |
| Phase                     | 0.01°/div, min                                                                                  |
| <b>Marker Resolution</b>  |                                                                                                 |
| Magnitude                 | 0.001 dB, min                                                                                   |
| Phase                     | 0.01°, min                                                                                      |
| Polar                     | 0.01 mUnit, min; 0.01°, min                                                                     |

**Table 23. Rear Panel Information**

| Description                                           | Supplemental Information |
|-------------------------------------------------------|--------------------------|
| <b>Test Port Bias Input</b>                           |                          |
| Connector                                             | BNC, female              |
| Maximum Voltage                                       | $\pm$ 30 VDC, typical    |
| Maximum Current (no degradation in RF specifications) | $\pm$ 200 mA, typical    |

|                              |                                                                                                                                                                                                                    |
|------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Maximum Current              | ±1 A, typical                                                                                                                                                                                                      |
| <b>Bias Input Connectors</b> |                                                                                                                                                                                                                    |
| Bias current                 | 500 mA, maximum                                                                                                                                                                                                    |
| Bias voltage                 | 40 Volts, maximum                                                                                                                                                                                                  |
| <b>10 MHz Reference In</b>   |                                                                                                                                                                                                                    |
| Connector                    | BNC, female                                                                                                                                                                                                        |
| Input Frequency              | 10 MHz ± 1 ppm, typical                                                                                                                                                                                            |
| Input Level                  | -15 dBm to +20 dBm, typical                                                                                                                                                                                        |
| Input Impedance              | 200 Ω, nom.                                                                                                                                                                                                        |
| <b>10 MHz Reference Out</b>  |                                                                                                                                                                                                                    |
| Connector                    | BNC, female                                                                                                                                                                                                        |
| Output Frequency             | 10 MHz ± 1 ppm, typical                                                                                                                                                                                            |
| Signal Type                  | Sine Wave, typical                                                                                                                                                                                                 |
| Output Level                 | +10 dBm ± 4 dB into 50 Ω, typical                                                                                                                                                                                  |
| Output Impedance             | 50 Ω, nominal                                                                                                                                                                                                      |
| Harmonics                    | <-40 dBc, typical                                                                                                                                                                                                  |
| <b>VGA Video Output</b>      |                                                                                                                                                                                                                    |
| Connector                    | 15-pin mini D-Sub; Drives VGA compatible monitors                                                                                                                                                                  |
| Devices Supported:           | Resolutions:                                                                                                                                                                                                       |
| Flat Panel (TFT)             | 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                                   |
| Flat Panel (DSTN)            | 800 X 600, 640 X 480                                                                                                                                                                                               |
| CRT Monitor                  | 1280 X 1024, 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                      |
|                              | Simultaneous operation of the internal and external displays is allowed, but with 640 X 480 resolution only. If you change resolution, you can only view the external display (internal display will "white out"). |
| <b>Test Set IO</b>           | 25-pin D-Sub connector, available for external test set control                                                                                                                                                    |
| <b>Aux IO</b>                | 25-pin D-Sub connector, male, analog and digital IO                                                                                                                                                                |
| <b>Handler IO</b>            | 36-pin IDC D-ribbon socket connector; all input/output signals are default set to negative logic; can be reset to positive logic via GPIB command                                                                  |
| <b>GPIB</b>                  | 24-pin D-sub (Type D-24), female; compatible with IEEE-488.                                                                                                                                                        |
| <b>Parallel Port (LPT1)</b>  | 25-pin D-Sub connector, female; provides connection to printers or any other parallel port peripheral                                                                                                              |

|                                  |                                                                                                |
|----------------------------------|------------------------------------------------------------------------------------------------|
| <b>Serial Port (COM 1)</b>       | 9-pin D-Sub, male; compatible with RS-232                                                      |
| <b>USB Port</b>                  |                                                                                                |
|                                  | Universal Serial Bus jack, Type A configuration (4 contacts inline, contact 1 on left); female |
| Contact 1                        | Vcc: 4.75 to 5.25 VDC, 500 mA, maximum                                                         |
| Contact 2                        | -Data                                                                                          |
| Contact 3                        | +Data                                                                                          |
| Contact 4                        | Ground                                                                                         |
| <b>LAN</b>                       | 10/100BaseT Ethernet; 8-pin configuration; auto selects between the two data rates             |
| <b>Line Power<sup>a, b</sup></b> |                                                                                                |
| Frequency at 110/115 V           | 50/60/400 Hz                                                                                   |
| Frequency at 230/240 V           | 50/60 Hz                                                                                       |
| Maximum Watts                    | 350 W                                                                                          |

**a** A third-wire ground is required.

**b** Power supply has a voltage autoswitching feature.

Note: Option H08 and Option H11 specifications are not provided in this E8356/7/8A specifications document.

**Table 24. Rear Panel Information (continued)**

| Description                    | Supplemental Information                                                                                                                                                                                                                                  |
|--------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>External AM Input</b>       |                                                                                                                                                                                                                                                           |
| Description                    | Input provides low-frequency AM modulation to test port output signal, or shifts the test port output. Zero volts input gives the power level set by the instrument, a positive voltage gives a higher level, and a negative voltage gives a lower level. |
| Connector                      | BNC, female                                                                                                                                                                                                                                               |
| Input Sensitivity              | 8 dB/V, typical                                                                                                                                                                                                                                           |
| Bandwidth                      | 1 kHz, typical                                                                                                                                                                                                                                            |
| Input Impedance                | 1 k $\Omega$ , typical                                                                                                                                                                                                                                    |
| <b>External Detector Input</b> |                                                                                                                                                                                                                                                           |
| Description                    | Input from an external, negative polarity diode detector provides ALC for a test port remote from instrument's front panel                                                                                                                                |
| Connector                      | BNC, female                                                                                                                                                                                                                                               |
| Input Sensitivity              | -500 mV yields approximately -3 dBm at detector's input, typical                                                                                                                                                                                          |
| Bandwidth                      | 50 kHz, typical                                                                                                                                                                                                                                           |
| Input Impedance                | 1 k $\Omega$ , nominal                                                                                                                                                                                                                                    |

**Table 25. Analyzer Environment and Dimensions**

| Description                                                                 | Supplemental Information                                                                                           |                    |                    |
|-----------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------|--------------------|--------------------|
| <b>General Environmental</b>                                                |                                                                                                                    |                    |                    |
| RFI/EMI Susceptibility                                                      | Defined by CISPR Pub. 11, Group 1, Class A, and IEC 50082-1                                                        |                    |                    |
| ESD                                                                         | Minimize using static-safe work procedures and an antistatic bench mat                                             |                    |                    |
| Dust                                                                        | Minimize for optimum reliability                                                                                   |                    |                    |
| <b>Operating Environment</b>                                                |                                                                                                                    |                    |                    |
| Temperature                                                                 | 0 °C to +40 °C<br>Instrument powers up, phase locks, and displays no error messages within this temperature range. |                    |                    |
| Error-Corrected Temperature Range                                           | 25°C ± 5°C<br>with less than 1°C deviation from calibration temp.                                                  |                    |                    |
| Humidity                                                                    | 5% to 95% at +40 °C                                                                                                |                    |                    |
| Altitude                                                                    | 0 to 4500 m (14,760 ft.)                                                                                           |                    |                    |
| <b>Non-Operating Storage Environment</b>                                    |                                                                                                                    |                    |                    |
| Temperature                                                                 | -40 °C to +70 °C                                                                                                   |                    |                    |
| Humidity                                                                    | 0% to 90% at +65 °C (non-condensing)                                                                               |                    |                    |
| Altitude                                                                    | 0 to 15,240 m (50,000 ft.)                                                                                         |                    |                    |
| <b>Cabinet Dimensions</b>                                                   |                                                                                                                    |                    |                    |
|                                                                             | Height                                                                                                             | Width              | Depth              |
| Excluding front and rear panel hardware and feet                            | 223 mm<br>8.75 in                                                                                                  | 426 mm<br>16.75 in | 427 mm<br>16.8 in  |
| As shipped - includes front panel connectors, rear panel bumpers, and feet. | 235 mm<br>9.25 in                                                                                                  | 435 mm<br>17.10 in | 470 mm<br>18.5 in  |
| As shipped plus handles                                                     | 235 mm<br>9.5 in                                                                                                   | 458 mm<br>18 in    | 501 mm<br>19.70 in |
| As shipped plus rack-mount flanges                                          | 235 mm<br>9.25 in                                                                                                  | 483 mm<br>19 in    | 470 mm<br>18.5 in  |
| As shipped plus handles and flanges                                         | 235 mm<br>9.25 in                                                                                                  | 483 mm<br>19 in    | 501 mm<br>19.70 in |
| <b>Weight</b>                                                               |                                                                                                                    |                    |                    |
| Net                                                                         | 24 kg (54 lb), nominal                                                                                             |                    |                    |
| Shipping                                                                    | 32 kg (70 lb), nominal                                                                                             |                    |                    |

Note: "Misc. Information" specifications are not included in this E8356/7/8A document.

## Measurement Throughput Summary

### Typical Cycle Time for Measurement Completion

#### Cycle Time with Changes in IF Bandwidth

#### Cycle Time with Changes in Number of Points

#### Data Transfer Time

#### Recall and Sweep Speed

**Table 26. Typical Cycle Time<sup>a,b</sup> (ms)**

|                                                       | Number of Points |     |     |      |
|-------------------------------------------------------|------------------|-----|-----|------|
|                                                       | 101              | 201 | 401 | 1601 |
| <b>Start 1.8 GHz, Stop 2 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected, 1-port cal                               | 9                | 12  | 18  | 54   |
| 2-Port cal                                            | 22               | 29  | 42  | 117  |
| <b>Start 300 kHz, Stop 3 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected, 1-port cal                               | 39               | 47  | 56  | 96   |
| 2-Port cal                                            | 80               | 101 | 121 | 204  |
| <b>Start 300 kHz, Stop 9 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected, 1-port cal                               | 51               | 57  | 64  | 103  |
| 2-Port cal                                            | 112              | 124 | 138 | 220  |

<sup>a</sup> Typical performance.

<sup>b</sup> Includes sweep time, retrace time and band-crossing time. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S11) measurement.

**Table 27. Cycle Time vs. IF Bandwidth<sup>a</sup>**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 1 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)



| IF Bandwidth (Hz) | Cycle Time (ms) <sup>b</sup> |
|-------------------|------------------------------|
| 40,000            | 8                            |
| 35,000            | 9                            |
| 30,000            | 11                           |
| 20,000            | 13                           |
| 10,000            | 28                           |
| 7000              | 36                           |
| 5000              | 48                           |
| 3000              | 72                           |
| 1000              | 196                          |
| 300               | 620                          |
| 100               | 1875                         |
| 30                | 8062                         |
| 10                | 17877                        |

**a** Typical performance.

**b** Cycle time includes sweep and retrace time.

### Table 28. Cycle Time vs. Number of Points<sup>a</sup>

Applies to the Preset condition (35 kHz IF bandwidth, correction off) except for the following changes:

- CF = 1 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Number of Points | Cycle Time (ms) <sup>b</sup> |
|------------------|------------------------------|
| 3                | 4                            |
| 11               | 4                            |
| 51               | 5                            |
| 101              | 6                            |
| 201              | 9                            |
| 401              | 16                           |
| 801              | 29                           |
| 1601             | 52                           |

**a** Typical performance.

**b** Cycle time includes sweep and retrace time.

### Table 29. Data Transfer Time<sup>a</sup> (ms)

|                                                                                   | Number of Points |     |     |      |
|-----------------------------------------------------------------------------------|------------------|-----|-----|------|
|                                                                                   | 51               | 201 | 401 | 1601 |
| <b>SCPI over GPIB<br/>(program executed on external PC)<sup>b</sup></b>           |                  |     |     |      |
| 32-bit floating point                                                             | 3                | 7   | 12  | 43   |
| 64-bit floating point                                                             | 4                | 12  | 22  | 84   |
| ASCII                                                                             | 7                | 64  | 124 | 489  |
| <b>SCPI over 100 Mbit/s LAN<br/>(program executed on external PC)<sup>b</sup></b> |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 1   | 1    |
| 64-bit floating point                                                             | 1                | 1   | 1   | 2    |
| ASCII                                                                             | 5                | 15  | 26  | 96   |
| <b>SCPI (program executed in the analyzer)<sup>d</sup></b>                        |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 2   | 3    |
| 64-bit floating point                                                             | 1                | 2   | 2   | 4    |
| ASCII                                                                             | 8                | 29  | 56  | 222  |
| <b>COM (program executed in the analyzer)<sup>e</sup></b>                         |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 1   | 1    |
| Variant type                                                                      | 1                | 1   | 2   | 6    |
| <b>DCOM over 100 Mbit/s LAN<br/>(program executed on external PC)<sup>f</sup></b> |                  |     |     |      |
| 32-bit floating point <sup>g</sup>                                                | 1                | 1   | 1   | 2    |
| Variant type <sup>h</sup>                                                         | 1                | 3   | 6   | 19   |

**a** Typical performance of unit with new 500 MHz Pentium III Processor.

**b** Measured using a VEE 5.0 program running on a 600 MHz HP Kayak, National Instruments<sup>TM</sup> GPIB card. Transferred complex S11 data, using "CALC:DATA?SDATA".

**c** Measured using a VEE 5.0 program running on a 600 MHz HP Kayak. Transferred complex S11 data, using "CALC:DATA?SDATA". Speed dependent on LAN traffic, if connected to network.

**d** Measured using a VEE 5.0 program running inside PNA Series Analyzer. Transferred complex S11 data, using "CALC:DATA?SDATA".

**e** Measured using a Visual Basic 6.0 program running inside PNA Series Analyzer. Transferred complex S11 data.

**f** Measured using a Visual Basic 6.0 program running on a 600 MHz HP Kayak. Transferred complex S11 data. Speed dependent on LAN traffic, if connected to network.

**g** Used IArray Transfer.getComplex method for 32-bit floating point.


**h** Used meas.getData method for Variant data type.

**Table 30. Recall and Sweep Speed<sup>a</sup>**


| Operations       | Number of Window(s) | Number of Trace(s) | Recall Time (ms) |
|------------------|---------------------|--------------------|------------------|
| Recall           | 1                   | 1                  | 49               |
| Recall and Sweep | 1                   | 1                  | 59               |
|                  |                     |                    |                  |
| Recall           | 1                   | 2                  | 82               |
| Recall and Sweep | 1                   | 2                  | 96               |
|                  |                     |                    |                  |
| Recall           | 1                   | 4                  | 159              |
| Recall and Sweep | 1                   | 4                  | 203              |
|                  |                     |                    |                  |
| Recall           | 2                   | 2                  | 93               |
| Recall and Sweep | 2                   | 2                  | 115              |
|                  |                     |                    |                  |
| Recall           | 3                   | 4                  | 158              |
| Recall and Sweep | 3                   | 4                  | 218              |
|                  |                     |                    |                  |
| Recall           | 4                   | 4                  | 187              |
| Recall and Sweep | 4                   | 4                  | 247              |
|                  |                     |                    |                  |
| Recall           | 4                   | 8                  | 340              |
| Recall and Sweep | 4                   | 8                  | 507              |

a CF= 177 MHz, Span = 200 MHz, 201 points, 35 kHz IF BW

**E8356A, E8357A, and E8358A – Simplified Test Set Block Diagram**

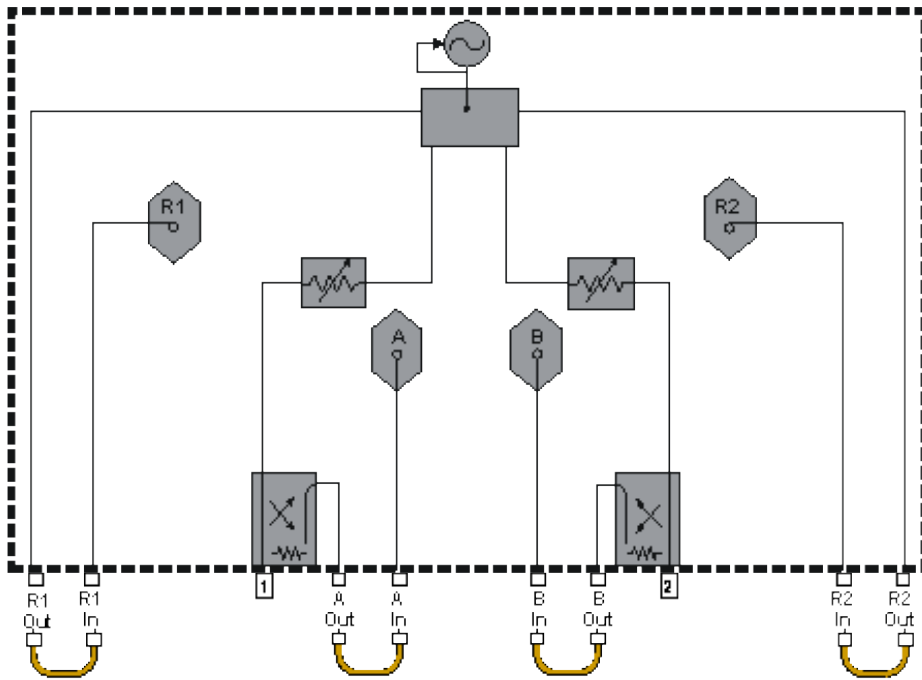

**E8356A, E8357A, and E8358A with Option 015 – Simplified Test Set Block Diagram**

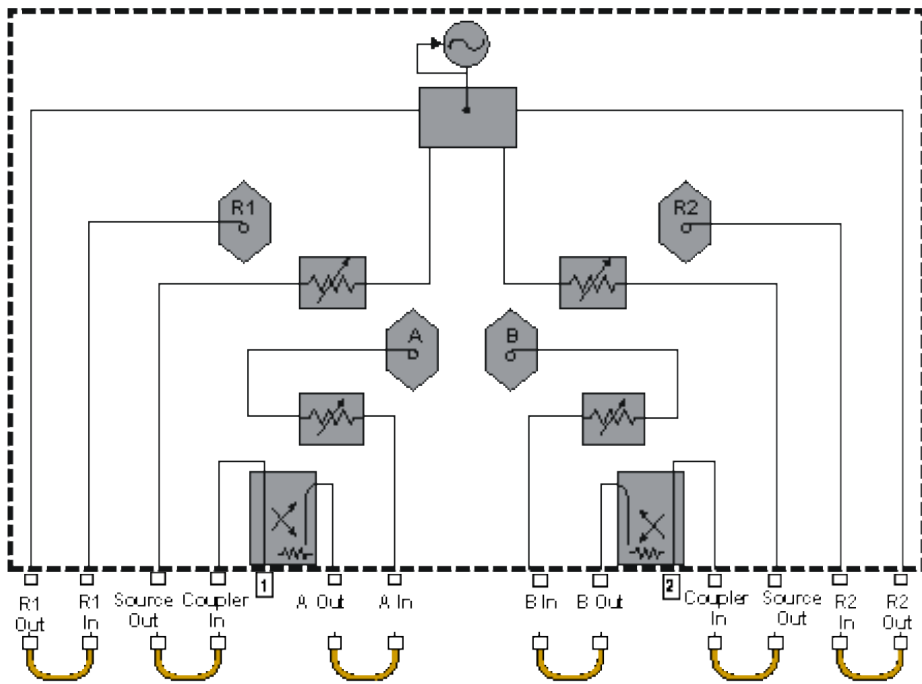

# Technical Specifications for the E8801A, E8802A, E8803A

(Rev. 2004-04-23)

This is a complete list of the E8801A, E8802A, and E8803A network analyzer technical specifications.

- To optimize viewing of uncertainty curves, click the Maximize button.
- To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "E880xA Specifications"
- The uncertainty curves contained in this document apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the [equations](#) used to generate the uncertainty curves.

---

## Definitions

### Corrected System Performance

#### System Dynamic Range

#### Type-N Connectors

#### 3.5 mm Connectors

#### 7-16 Connectors

### Uncorrected Instrument Performance

#### Test Port Output Characteristics (Source)

#### Test Port and Receiver Input Characteristics

### General Information

#### Front-panel Jumper Specs (Option 014 only)

#### Measurement Throughput Summary

#### Test Set Block Diagram

#### Test Set with Option 015 Block Diagram

[See Specs for other PNA models](#)

## Definitions

All specifications and characteristics apply over a 25 °C ±5 °C range (unless otherwise stated) and 90 minutes after the instrument has been turned on.

**Specification (spec.):** Warranted performance. Specifications include guardbands to account for the expected statistical performance distribution, measurement uncertainties, and changes in performance due to environmental

conditions.

**Characteristic (char.):** A performance parameter that the product is expected to meet before it leaves the factory, but that is not verified in the field and is not covered by the product warranty. A characteristic includes the same guardbands as a specification.

**Typical (typ.):** Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Nominal (nom.):** A general, descriptive term that does not imply a level of performance. It is not covered by the product warranty.

**Calibration:** The process of measuring known standards to characterize a network analyzer's systematic (repeatable) errors.

**Corrected (residual):** Indicates performance after error correction (calibration). It is determined by the quality of calibration standards and how well "known" they are, plus system repeatability, stability, and noise.

**Uncorrected (raw):** Indicates instrument performance without error correction. The uncorrected performance affects the stability of a calibration.

**Standard:** When referring to the analyzer, this includes no options unless noted otherwise.

---

## Corrected System Performance

The specifications in this section apply for measurements made with the E8801A, E8802A, and E8803A analyzer with the following conditions:

- 10 Hz IF bandwidth
- No averaging applied to data
- Environmental temperature of 25 °C ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted

---

**Note:** The uncertainty curves contained in these specifications apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the equations used to generate the uncertainty curves.

---

### System Dynamic Range

#### Type-N Connectors

#### 3.5 mm Connectors

#### 7/16 Connectors

## Table 1. System Dynamic Range

| Description                                          | Specification (dB) | Characteristic (dB) |
|------------------------------------------------------|--------------------|---------------------|
| <b>Dynamic range<sup>a</sup> (at test port)</b>      |                    |                     |
| 300 kHz to 25 MHz <sup>b</sup>                       | 125                |                     |
| 25 MHz to 3 GHz <sup>b</sup>                         | 128                |                     |
| 3 GHz to 6 GHz                                       | 118                |                     |
| 6 GHz to 9 GHz                                       | 115                |                     |
| <b>Dynamic range<sup>c</sup> (at receiver input)</b> |                    |                     |
| 300 kHz to 25 MHz <sup>d</sup>                       |                    | 140                 |
| 25 MHz to 3 GHz <sup>d</sup>                         |                    | 143                 |
| 3 GHz to 6 GHz                                       |                    | 133                 |
| 6 GHz to 9 GHz                                       |                    | 130                 |

**a** The test port dynamic range is calculated as the difference between the test port rms noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account.

**b** May be limited to 100 dB at particular frequencies below 750 MHz due to spurious receiver residuals.

**c** The receiver input dynamic range is calculated as the difference between the receiver rms noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its damage level. When the analyzer is in segment sweep mode, frequency segments can be defined with a higher power level when the extended dynamic range is required (i.e. the portion of the device's response with high insertion loss), and reduced power when receiver damage may occur (i.e. the portion of the device's response with low insertion loss).

**d** May be limited to 115 dB at particular frequencies below 750 MHz due to spurious receiver residuals.

**Note:** Receiver Dynamic Range specifications are not included in this E8801/2/3A document.

## Corrected System Performance with Type-N Connectors

### 85032F Calibration Kit

### 85092C Electronic Calibration Module

---

**Note:** This document provides technical specifications for the following calibration kits only: 85032F, 85092C, 85033E, 85093C and 85038A.

---



## Table 2. Corrected System Performance With Type-N Device Connectors, 85032F Calibration Kit

Applies to the E8801A, E8802A, and E8803A analyzer, 85032F (Type-N, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:



- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted

| Description           | Specification (dB) |                  |                |               |
|-----------------------|--------------------|------------------|----------------|---------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 GHz to 6 GHz | 6GHz to 9 GHz |
| Directivity           | 49                 | 46               | 40             | 38            |
| Source Match          | 41                 | 40               | 36             | 35            |
| Load Match            | 49                 | 45               | 39             | 37            |
| Reflection Tracking   | $\pm 0.011$        | $\pm 0.021$      | $\pm 0.032$    | $\pm 0.054$   |
| Transmission Tracking | $\pm 0.012$        | $\pm 0.020$      | $\pm 0.055$    | $\pm 0.083$   |

### Transmission Uncertainty (Specifications)

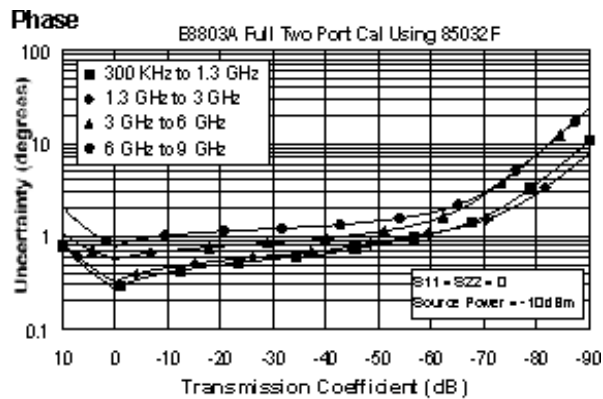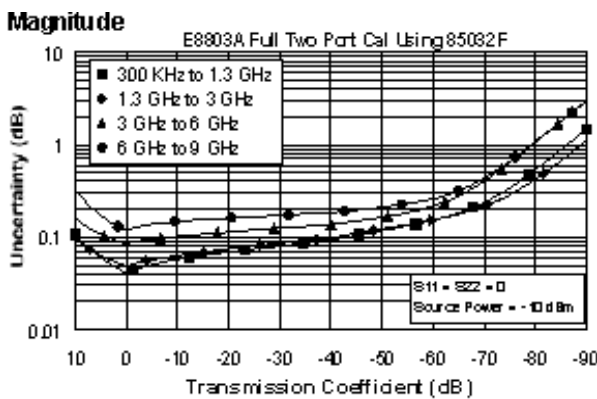

### Reflection Uncertainty (Specifications)

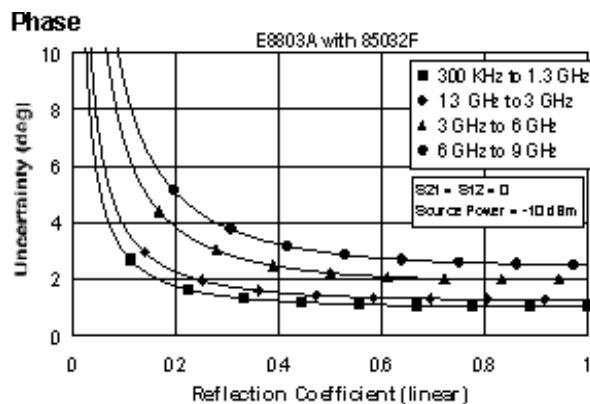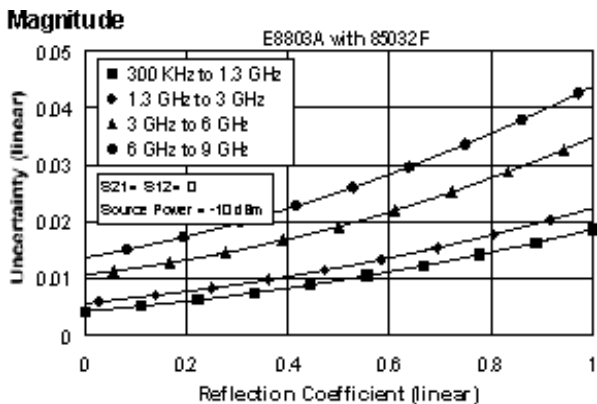

**Table 3. Corrected System Performance With Type-N Device Connectors, 85092C Electronic Calibration Module**

Applies to the E8801A, E8802A, and E8803A analyzer, 85092C (Type-N, 50 $\Omega$ ) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:


- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25°  $\pm$ 5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted




| Description           | Specification (dB) |                  |                |                         |
|-----------------------|--------------------|------------------|----------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 GHz to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 54               | 52             | 47                      |
| Source Match          | 45                 | 44               | 41             | 36                      |
| Load Match            | 47                 | 47               | 44             | 39                      |
| Reflection Tracking   | ±0.040             | ±0.040           | ±0.060         | ±0.070                  |
| Transmission Tracking | ±0.039             | ±0.039           | ±0.068         | ±0.136                  |

### Transmission Uncertainty (Specifications)

#### Magnitude

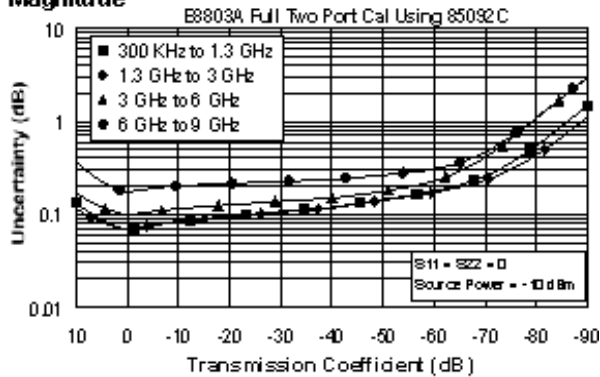


#### Phase

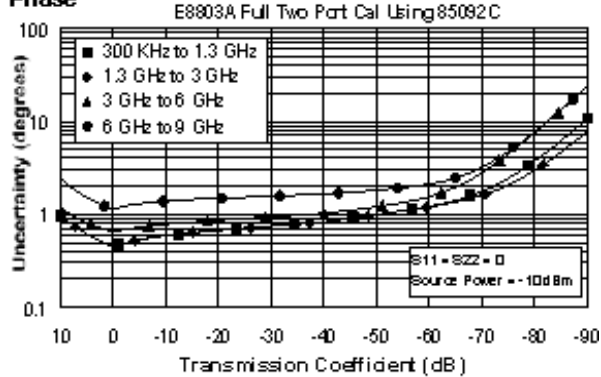


### Reflection Uncertainty (Specifications)

#### Magnitude

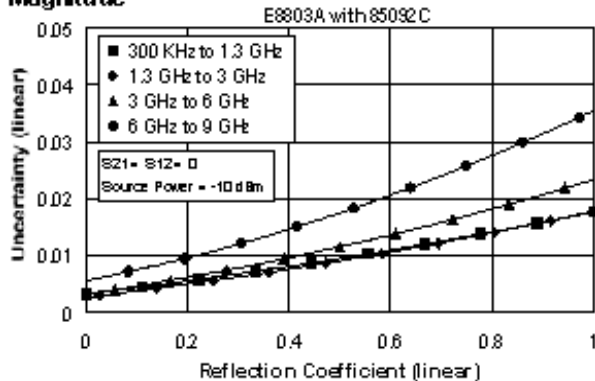

#### Phase

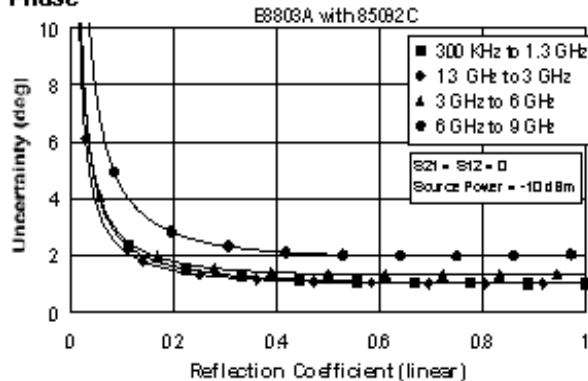

### Corrected System Performance with 3.5 mm Connectors

[85033E Calibration Kit](#)

[85093C Electronic Calibration Module](#)

**Table 4. Corrected System Performance With 3.5 mm Device Connector Type, 85033E Calibration Kit**


Applies to the E8801A, E8802A, and E8803A analyzer, 85033E (3.5 mm, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |                |                |
|-----------------------|--------------------|------------------|----------------|----------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 GHz to 6 GHz | 6 GHz to 9 GHz |
| Directivity           | 46                 | 44               | 38             | 38             |
| Source Match          | 43                 | 40               | 37             | 36             |
| Load Match            | 46                 | 44               | 38             | 38             |
| Reflection Tracking   | ±0.006             | ±0.007           | ±0.009         | ±0.010         |
| Transmission Tracking | ±0.012             | ±0.021           | ±0.057         | ±0.075         |

### Transmission Uncertainty (Specifications)

#### Magnitude

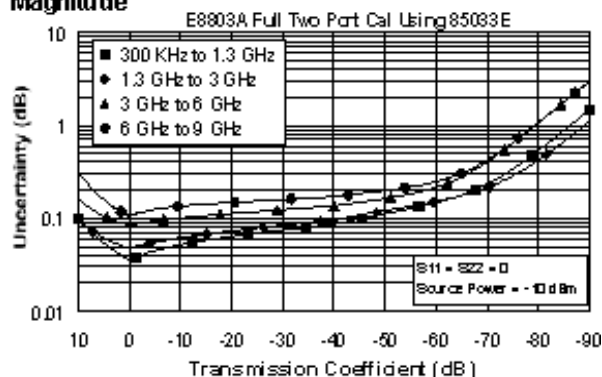


#### Phase

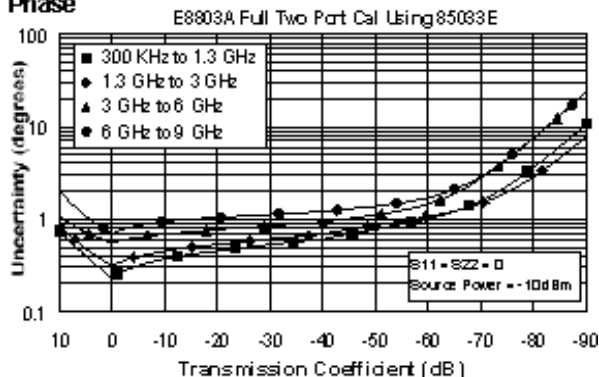


### Reflection Uncertainty (Specifications)

#### Magnitude

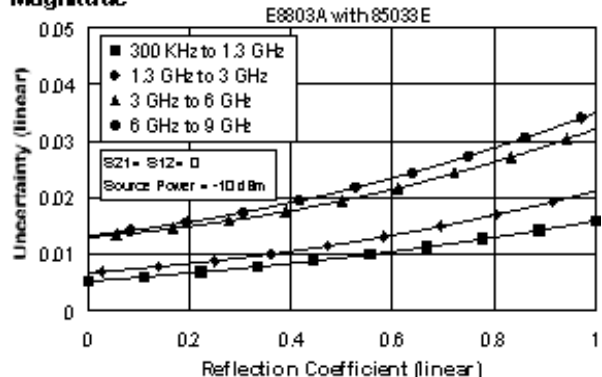

#### Phase

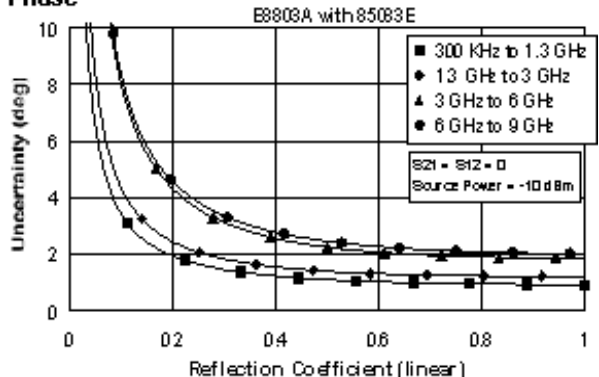

**Table 5. Corrected System Performance With 3.5 mm Device Connector Type, 85093C Electronic Calibration Module**

Applies to the E8801A, E8802A, and E8803A analyzer, 85093C (3.5 mm, 50Ω) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:


- IF bandwidth = 10 Hz

- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |                |                             |
|-----------------------|--------------------|------------------|----------------|-----------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 GHz to 6 GHz | 6 GHz to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 52               | 51             | 47                          |
| Source Match          | 44                 | 44               | 39             | 34                          |
| Load Match            | 47                 | 47               | 44             | 40                          |
| Reflection Tracking   | ±0.030             | ±0.040           | ±0.050         | ±0.070                      |
| Transmission Tracking | ±0.039             | ±0.049           | ±0.068         | ±0.117                      |

### Transmission Uncertainty (Specifications)

#### Magnitude

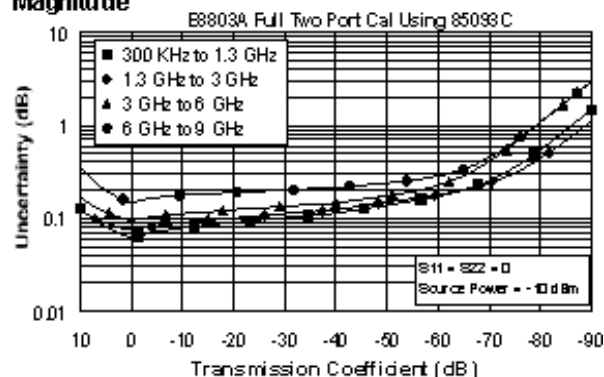


#### Phase

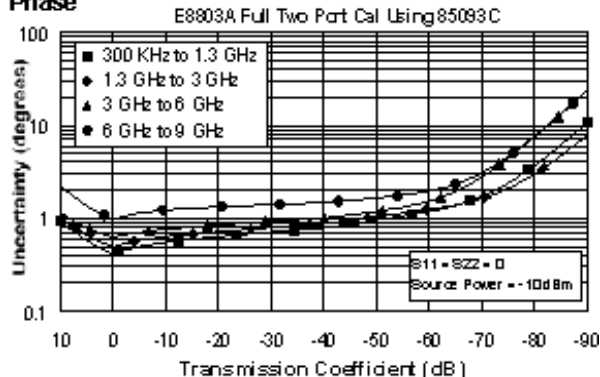


### Reflection Uncertainty (Specifications)

#### Magnitude

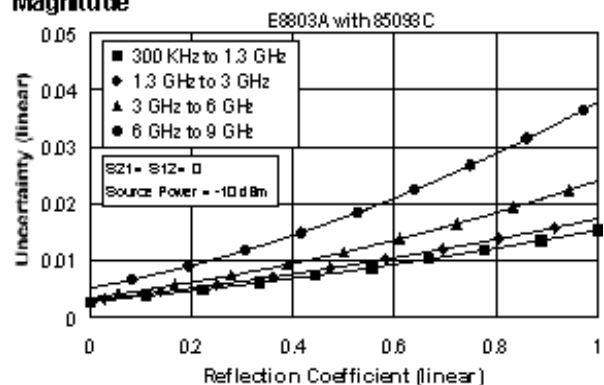

#### Phase

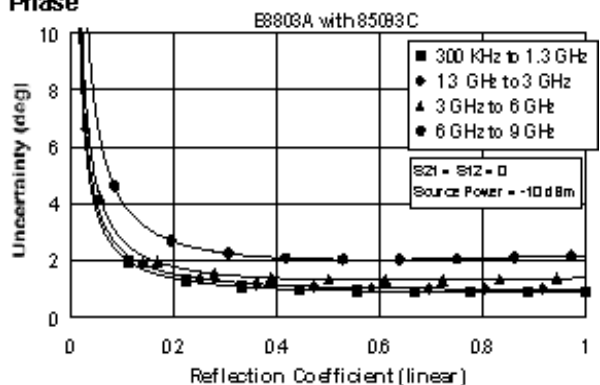

**Table 6. Corrected System Performance With 7-16 Device Connector Type, 85038A Calibration Kit**

Applies to the E8801A, E8802A, and E8803A analyzer, 85038A (7-16, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:


- IF bandwidth = 10 Hz
- No averaging applied to data

- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 40                 | 40               | 36         | 36                      |
| Source Match          | 37                 | 37               | 34         | 34                      |
| Load Match            | 39                 | 39               | 35         | 35                      |
| Reflection Tracking   | ±0.089             | ±0.089           | ±0.115     | ±0.115                  |
| Transmission Tracking | ±0.024             | ±0.033           | ±0.082     | ±0.103                  |

### Transmission Uncertainty (Specifications)

#### Magnitude

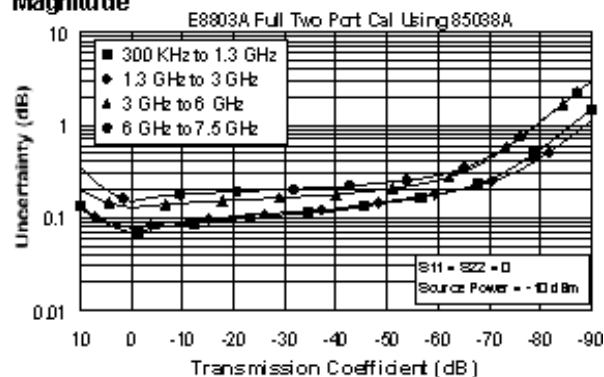


#### Phase

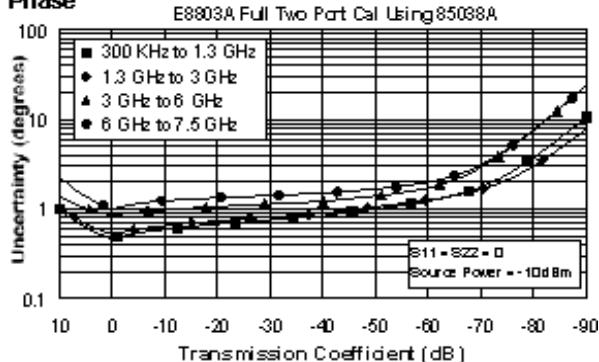

### Reflection Uncertainty (Specifications)

#### Magnitude

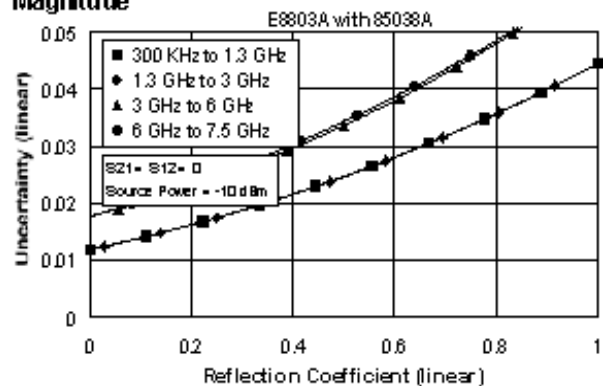

#### Phase

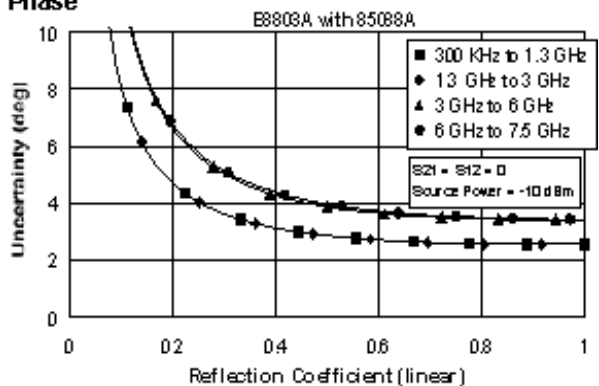


Table 7. Uncorrected Instrument Performance

| Description           | Specification (dB) |                 |                  |                |                |
|-----------------------|--------------------|-----------------|------------------|----------------|----------------|
|                       | 300 kHz to 1 MHz   | 1MHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 GHz to 6 GHz | 6 GHz to 9 GHz |
| Directivity           | 30                 | 33              | 27               | 20             | 13             |
| Source Match          | 18                 | 18              | 16               | 11             | 8              |
| Load Match            | 20                 | 20              | 17               | 13.5           | 13             |
| Reflection Tracking   | ±1.5               | ±1.5            | ±1.5             | ±2.5           | ±3.0           |
| Transmission Tracking | ±1.5               | ±1.5            | ±1.5             | ±2.5           | ±3.0           |

### Test Port Output Characteristics (Source)

Output Frequency

Output Power

Output Signal Purity

**Table 8. Test Port Output Frequency**

| Description                          | Specification      | Supplemental Information                                 |
|--------------------------------------|--------------------|----------------------------------------------------------|
| <b>Range:</b>                        |                    |                                                          |
| E8801A                               | 300 kHz to 3.0 GHz |                                                          |
| E8802A                               | 300 kHz to 6.0 GHz |                                                          |
| E8803A                               | 300 kHz to 9.0 GHz |                                                          |
| <b>Resolution:</b>                   | 1 Hz               |                                                          |
| <b>Source Stability</b>              |                    | ±1 ppm, 0°C to 40 °C, typical<br>±1ppm/year maximum      |
| <b>Source Stability (Option 1E5)</b> |                    | ±0.05 ppm, 0° to 70 °C, typical<br>±0.1 ppm/year maximum |
| <b>CW Accuracy</b>                   | ±3 ppm             |                                                          |
| <b>CW Accuracy (Option 1E5)</b>      | ±1 ppm             |                                                          |

**Table 9. Test Port Output Power<sup>a</sup>**

| Description               | Specification  | Supplemental Information              |
|---------------------------|----------------|---------------------------------------|
| <b>Level Accuracy:</b>    |                |                                       |
| 300 kHz to 6 GHz          | ±1.0 dB        | Variation from 0 dBm in power range 0 |
| 6 GHz to 9 GHz            | ±2.0 dB        | ±1.5dB below 10 MHz                   |
| <b>Level Linearity:</b>   |                |                                       |
|                           |                | Variation from 0 dBm in power range 0 |
| 300 kHz to 9 GHz          | ±0.3 dB        | -15 to +5 dBm                         |
| 300 kHz to 1 MHz          | ±1.0 dB        | +5 to +10 dBm                         |
| 1 MHz to 6 GHz            | ±0.5 dB        | +5 to +10 dBm                         |
| 6 GHz to 9 GHz            | ±0.5 dB        | +5 to +7 dBm                          |
| <b>Range<sup>b</sup>:</b> |                |                                       |
| 300 kHz to 6 GHz          | -15 to +10 dBm |                                       |
| 6 GHz to 9 GHz            | -15 to +7 dBm  |                                       |
| <b>Range<sup>b</sup>:</b> |                |                                       |
| (Option 1E1):             |                |                                       |
| 300 kHz to 6 GHz          | -85 to +10 dBm |                                       |
| 6 GHz to 9 GHz            | -85 to +7 dBm  |                                       |
| <b>Sweep Range</b>        |                |                                       |
| 300 kHz to 6 GHz          | 25 dB          |                                       |
| 6 GHz to 9 GHz            | 22 dB          |                                       |
| <b>Level Resolution</b>   | 0.01 dB        |                                       |

<sup>a</sup> Source output performance on port 1 only. Port 2 output performance is typical.

<sup>b</sup> Power to which the source can be set and phase lock is assured.

**Table 10. Test Port Output Signal Purity**

| Description                           | Specification | Supplemental Information               |
|---------------------------------------|---------------|----------------------------------------|
| <b>Harmonics (2nd or 3rd)</b>         |               |                                        |
| at max output power (< 25 MHz)        |               | < -25 dBc, typical                     |
| at max output power (25 MHz to 9 GHz) |               | < -25 dBc, characteristic <sup>a</sup> |
| at 0 dBm output                       |               | < -35 dBc, typical                     |
| at -10 dBm output                     |               | < -38 dBc, typical, in power range 0   |
| <b>Non-harmonic Spurious</b>          |               |                                        |
| at max output                         |               | -30 dBc, typical for offset freq>1kHz  |
| at -10 dBm output                     |               | -50 dBc, typical for offset freq >1kHz |

<sup>a</sup> Typical below 25 MHz.

## Test Port and Receiver Input Characteristics

### Input Levels

### Trace Noise

### Reference Level and Stability

### Dynamic Accuracy

### Group Delay

**Table 11. Test Port and Receiver Input Levels**

| Description                          | Specification | Supplemental Information |
|--------------------------------------|---------------|--------------------------|
| <b>Maximum Test Port Input Level</b> |               |                          |
| Test Ports 1 and 2:                  |               |                          |
| 300 kHz to 25 MHz                    | +10 dBm       | < 0.6 dB compression     |
| 25 MHz to 3 GHz                      | +10 dBm       | < 0.4 dB compression     |
| 3 GHz to 6 GHz                       | +10 dBm       | < 0.7 dB compression     |
| 6 GHz to 9 GHz                       | +5 dBm        | < 0.7 dB compression     |
| <b>Damage Level</b>                  |               |                          |
| Test Port 1, 2                       |               | +30 dBm or ±30 VDC, typ. |
| R, A, B (Opt. 014)                   |               | +15 dBm or ±5 VDC, typ.  |
| Coupler Thru (Opt. 014)              |               | +33 dBm or ±0 VDC, typ.  |

| <b>Test Port Noise Floor<sup>a</sup></b>      |            |                                                               |
|-----------------------------------------------|------------|---------------------------------------------------------------|
| 300 kHz to 25 MHz <sup>b</sup>                |            |                                                               |
| 10 Hz IF Bandwidth                            | -115 dBm   |                                                               |
| 1 kHz IF Bandwidth                            | -95 dBm    |                                                               |
| 25 MHz to 3 GHz <sup>b</sup>                  |            |                                                               |
| 10 Hz IF Bandwidth                            | -118 dBm   |                                                               |
| 1 kHz IF Bandwidth                            | -98 dBm    |                                                               |
| 3 GHz to 9 GHz                                |            |                                                               |
| 10 Hz IF Bandwidth                            | ≤ -108 dBm |                                                               |
| 1 kHz IF Bandwidth                            | ≤ -88 dBm  |                                                               |
| <b>Receiver Noise Floor<sup>a</sup></b>       |            |                                                               |
| 300 kHz to 25 MHz <sup>c</sup>                |            |                                                               |
| 10 Hz IF Bandwidth                            | ≤ -130 dBm |                                                               |
| 1 kHz IF Bandwidth                            | ≤ -110 dBm |                                                               |
| 25 MHz to 3 GHz <sup>c</sup>                  |            |                                                               |
| 10 Hz IF Bandwidth                            | ≤ -133 dBm |                                                               |
| 1 kHz IF Bandwidth                            | ≤ -113 dBm |                                                               |
| 6 GHz to 9 GHz                                |            |                                                               |
| 10 Hz IF Bandwidth                            | ≤ -123 dBm |                                                               |
| 1 kHz IF Bandwidth                            | ≤ -103 dBm |                                                               |
| <b>Crosstalk</b>                              |            |                                                               |
|                                               |            | Between test ports 1 and 2, with short circuits at both ports |
| 300 kHz to 1 MHz                              | <-120 dB   |                                                               |
| 1 MHz to 25 MHz                               | <-125 dB   |                                                               |
| 25 MHz to 3 GHz                               | <-126 dB   |                                                               |
| 3 GHz to 6 GHz                                | <-117 dB   |                                                               |
| 6 GHz to 9 GHz                                | <-106 dB   |                                                               |
| <b>Maximum Receiver Input Level (A, B, R)</b> |            |                                                               |



|                                              |  |                         |
|----------------------------------------------|--|-------------------------|
| 300 kHz to 6 GHz                             |  | -6 dBm, typical         |
| 6 GHz to 9 GHz                               |  | -9 dBm, typical         |
| <b>Reference Input Level (R)<sup>d</sup></b> |  |                         |
| 300 kHz to 9 GHz                             |  | -10 to -35 dBm, typical |
| <b>Maximum Coupler Input Level (Opt 014)</b> |  |                         |
| 300 kHz to 9 GHz                             |  | +33 dBm, typical        |

**a** Total average (RMS) noise power calculated as the mean value of a linear magnitude trace expressed in dBm.

**b** May be limited to -90 dBm at particular frequencies below 750 MHz due to spurious receiver residuals.

**c** May be limited to -105 dBm at particular frequencies below 750 MHz due to spurious receiver residuals.

**d** Input level to maintain phase lock.

**Table 12. Test Port Input (Trace Noise)**

| Description                              | Specification  | Supplemental Information |
|------------------------------------------|----------------|--------------------------|
| <b>Trace Noise<sup>a</sup> Magnitude</b> |                |                          |
| 1 kHz IF Bandwidth                       | < 0.002 dB rms |                          |
| 10 kHz IF Bandwidth                      | < 0.005 dB rms |                          |
| <b>Trace Noise<sup>a</sup> Phase</b>     |                |                          |
| 1 kHz IF Bandwidth                       | < 0.010° rms   |                          |
| 10 kHz IF Bandwidth                      | < 0.035° rms   |                          |

**a** Trace noise is defined as a ratio measurement of a through or a full reflection, with the source set to 0 dBm.

**Table 13. Test Port Input (Reference Level and Stability)**

| Description                            | Specification | Supplemental Information |
|----------------------------------------|---------------|--------------------------|
| <b>Reference Level Magnitude</b>       |               |                          |
| Range                                  | ±200 dB       |                          |
| Resolution                             | 0.001 dB      |                          |
| <b>Reference Level Phase</b>           |               |                          |
| Range                                  | ±500°         |                          |
| Resolution                             | 0.01°         |                          |
| <b>Stability Magnitude<sup>a</sup></b> |               |                          |
| 300 kHz to 3 GHz                       |               | 0.02 dB/°C, typical      |
| 3 GHz to 6 GHz                         |               | 0.04 dB/°C, typical      |
| 6 GHz to 9 GHz                         |               | 0.06 dB/°C, typical      |
| <b>Stability Phase<sup>a</sup></b>     |               |                          |
| 300 kHz to 3 GHz                       |               | 0.2°/°C, typical         |
| 3 GHz to 6 GHz                         |               | 0.3°/°C, typical         |
| 6 GHz to 9 GHz                         |               | 0.6°/°C, typical         |


a Stability is defined as a ratio measurement at the test port.

**Table 14. Test Port Input (Dynamic Accuracy specification<sup>a</sup>)**


Accuracy of the test port input power reading is relative to the reference input power level. Applies to input ports 1 and 2 with the following conditions:

- IF bandwidth = 10 Hz
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature


300 kHz to 3 GHz

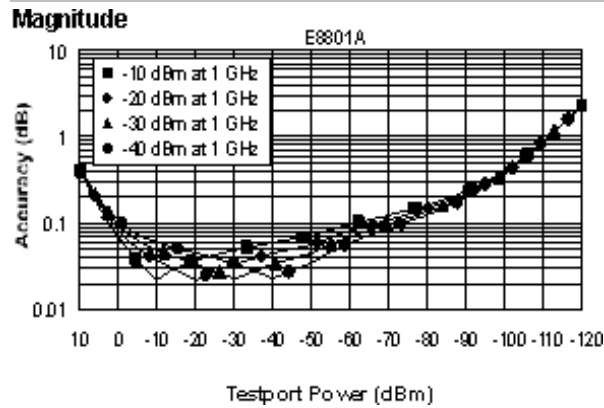


300 kHz to 3 GHz

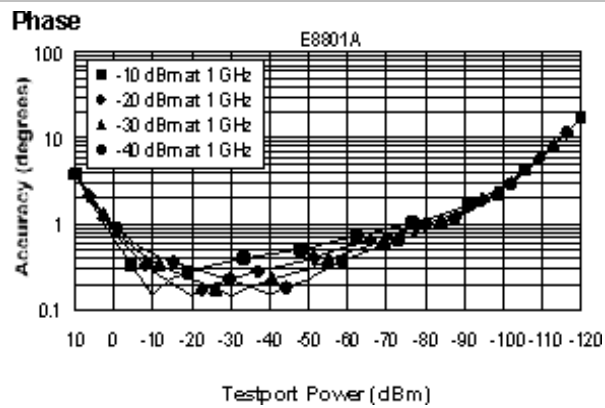


300 kHz to 6 GHz

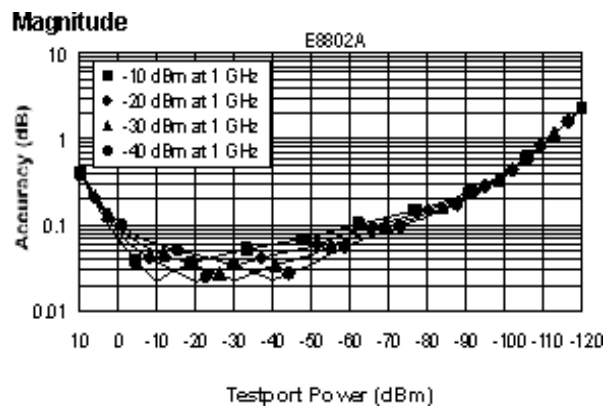


300 kHz to 6 GHz

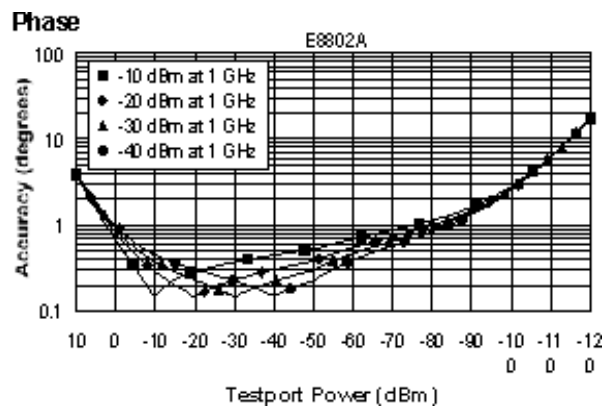

300 kHz to 9 GHz

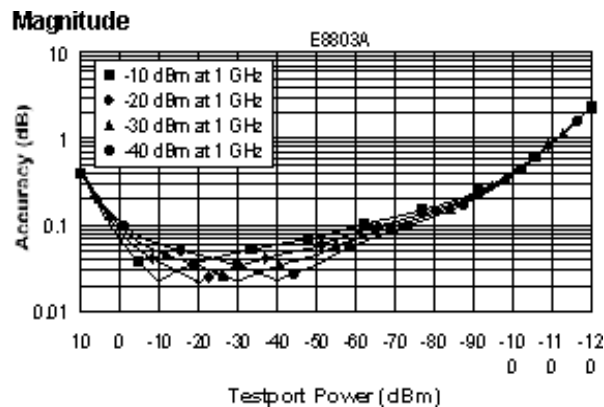

300 kHz to 9 GHz

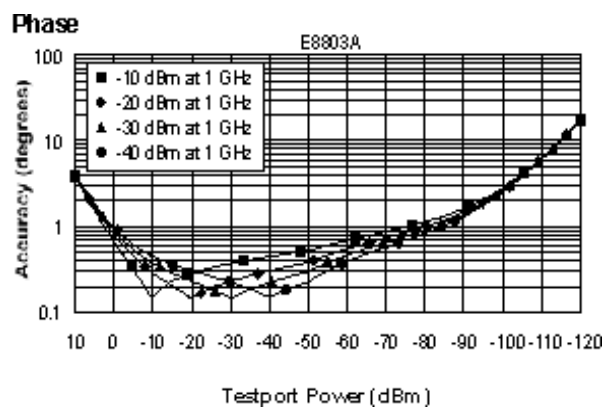


a Dynamic accuracy is verified with the following measurements:

- compression over frequency
- IF linearity at a single frequency of 1.195 GHz and a reference level of -20 dBm

**Table 15. Test Port Input (Group Delay)<sup>a</sup>**

| Description           | Specification                           | Supplemental Information                                                             |
|-----------------------|-----------------------------------------|--------------------------------------------------------------------------------------|
| Aperture (selectable) | (frequency span)/(number of points - 1) |                                                                                      |
| Maximum Aperture      | 20% of frequency span                   |                                                                                      |
| Range                 | 0.5 x (1/minimum aperture)              |                                                                                      |
| Maximum Delay         |                                         | Limited to measuring no more than 180° of phase change within the minimum aperture.) |
| Accuracy              |                                         | See graph below. Char.                                                               |

The following graph shows group delay accuracy with type-N full 2-port calibration and a 10 Hz IF bandwidth. Insertion loss is assumed to be < 2 dB and electrical length to be ten meters.

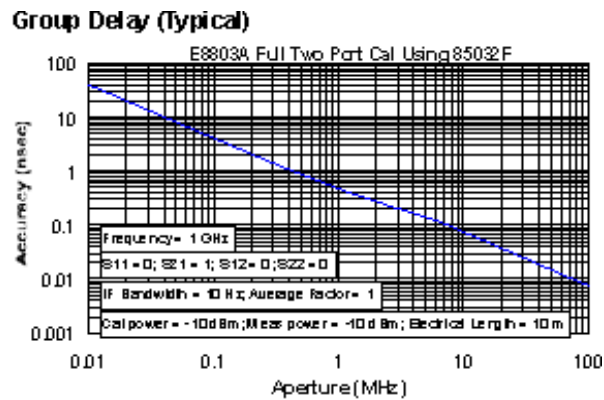

In general, the following formula can be used to determine the accuracy, in seconds, of specific group delay measurement:

$$\pm \text{Phase Accuracy (deg)} / [360 \times \text{Aperture (Hz)}]$$

Depending on the aperture and device length, the phase accuracy used is either incremental phase accuracy or worst case phase accuracy.

a Group delay is computed by measuring the phase change within a specified frequency step (determined by the frequency span and the number of points per sweep).

## General Information

### [System Bandwidths](#)

### [Front Panel](#)

### [Rear Panel](#)

### [Environment and Dimensions](#)

## Table 16. System Bandwidths

| Description                  | Specification | Supplemental Information                                                              |
|------------------------------|---------------|---------------------------------------------------------------------------------------|
| <b>IF Bandwidth Settings</b> |               |                                                                                       |
| Range                        |               | 1 Hz to 40 kHz<br>in a 1, 2, 3, 5, 7,10 sequence up to 30 kHz, 35 kHz, 40kHz, nominal |

**Table 17. Front Panel Information**

| Description               | Supplemental Information                                                                        |
|---------------------------|-------------------------------------------------------------------------------------------------|
| <b>RF Connectors</b>      |                                                                                                 |
| Type                      | Type-N, female; 50 $\Omega$ , nominal                                                           |
| Center Pin Protrusion     | 0.204 to 0.207 in., characteristic                                                              |
| <b>Probe Power</b>        |                                                                                                 |
| Connector                 | 3-pin connector, male                                                                           |
| Positive Supply           | +15 VDC $\pm$ 2%, 400 mA, max, characteristic                                                   |
| Negative Supply           | -12.6 VDC $\pm$ 5%, 300 mA, max, characteristic                                                 |
| <b>Display</b>            |                                                                                                 |
| Size                      | 21.3 cm (8.4 in) diagonal color active matrix LCD; 640 (horizontal) X 480 (vertical) resolution |
| Refresh Rate              | Vertical 59.83 Hz; Horizontal 31.41 Hz                                                          |
| <b>Display Range</b>      |                                                                                                 |
| Magnitude                 | $\pm$ 200 dB (at 20 dB/div), max                                                                |
| Phase                     | $\pm$ 180°, max                                                                                 |
| Polar                     | 10 pUnits, min<br>1000 Units, max                                                               |
| <b>Display Resolution</b> |                                                                                                 |
| Magnitude                 | 0.001 dB/div, min                                                                               |
| Phase                     | 0.01°/div, min                                                                                  |
| <b>Marker Resolution</b>  |                                                                                                 |
| Magnitude                 | 0.001 dB, min                                                                                   |
| Phase                     | 0.01°, min                                                                                      |
| Polar                     | 0.01 mUnit, min; 0.01°,min                                                                      |

**Table 18. Rear Panel Information**

| Description                | Supplemental Information |
|----------------------------|--------------------------|
| <b>10 MHz Reference In</b> |                          |

|                             |                                                                                                                                                                                                                    |
|-----------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Connector                   | BNC, female                                                                                                                                                                                                        |
| Input Frequency             | 10 MHz $\pm$ 1 ppm, typical                                                                                                                                                                                        |
| Input Level                 | -15 dBm to +20 dBm, typical                                                                                                                                                                                        |
| Input <u>Impedance</u>      | 200 $\Omega$ , nom.                                                                                                                                                                                                |
| <b>10 MHz Reference Out</b> |                                                                                                                                                                                                                    |
| Connector                   | BNC, female                                                                                                                                                                                                        |
| Output Frequency            | 10 MHz $\pm$ 10 ppm, typical                                                                                                                                                                                       |
| Signal Type                 | Sine Wave, typical                                                                                                                                                                                                 |
| Output Level                | +10 dBm $\pm$ 4 dB into 50 $\Omega$ , typical                                                                                                                                                                      |
| Output Impedance            | 50 $\Omega$ , nominal                                                                                                                                                                                              |
| Harmonics                   | <-40 dBc, typical                                                                                                                                                                                                  |
| <b>VGA Video Output</b>     |                                                                                                                                                                                                                    |
| Connector                   | 15-pin mini D-Sub; Drives VGA compatible monitors                                                                                                                                                                  |
| Devices Supported           | Resolutions                                                                                                                                                                                                        |
| Flat Panel (TFT             | 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                                   |
| Flat Panel (DSTN)           | 800 X 600, 640 X 480                                                                                                                                                                                               |
| CRT Monitor                 | 1280 X 1024, 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                      |
|                             | Simultaneous operation of the internal and external displays is allowed, but with 640 X 480 resolution only. If you change resolution, you can only view the external display (internal display will "white out"). |
| <b>Test Set IO</b>          | 25-pin D-Sub connector, available for external test set control                                                                                                                                                    |
| <b>Aux IO</b>               | 25-pin D-Sub connector, male, analog and digital IO                                                                                                                                                                |
| <b>Handler IO</b>           | 36-pin IDC D-ribbon socket connector; all input/output signals are default set to negative logic; can be reset to positive logic via GPIB command                                                                  |
| <b>GPIB</b>                 | 24-pin D-sub (Type D-24), female; compatible with IEEE-488.                                                                                                                                                        |
| <b>Parallel Port (LPT1)</b> | 25-pin D-Sub connector, female; provides connection to printers or any other parallel port peripherals                                                                                                             |
| <b>Serial Port (COM 1)</b>  | 9-pin D-Sub, male; compatible with RS-232                                                                                                                                                                          |
| <b>USB Port</b>             |                                                                                                                                                                                                                    |
|                             | Universal Serial Bus jack, Type A configuration (4 contacts inline, contact 1 on left); female                                                                                                                     |
| Contact 1                   | Vcc: 4.75 to 5.25 VDC, 500 mA, maximum                                                                                                                                                                             |

|                                  |                                                                                    |
|----------------------------------|------------------------------------------------------------------------------------|
| Contact 2                        | -Data                                                                              |
| Contact 3                        | +Data                                                                              |
| Contact 4                        | Ground                                                                             |
| <b>LAN</b>                       | 10/100BaseT Ethernet, 8-pin configuration; auto selects between the two data rates |
| <b>Line Power<sup>a, b</sup></b> |                                                                                    |
| Frequency at 110/115 V           | 50/60/400 Hz                                                                       |
| Frequency at 230/240 V           | 50/60 Hz                                                                           |
| Maximum Watts                    | 350 W                                                                              |

**a** A third-wire ground is required.

**b** Power supply has a voltage autoswitching feature.

Note: Option H08 and Option H11 specifications are not provided in this E8801/2/3A specifications document.

**Table 19. Rear Panel Information (continued)**

| Description                    | Supplemental Information                                                                                                                                                                                                                                  |
|--------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>External AM Input</b>       |                                                                                                                                                                                                                                                           |
| Description                    | Input provides low-frequency AM modulation to test port output signal, or shifts the test port output. Zero volts input gives the power level set by the instrument, a positive voltage gives a higher level, and a negative voltage gives a lower level. |
| Connector                      | BNC, female                                                                                                                                                                                                                                               |
| Input Sensitivity              | 8 dB/V, typical                                                                                                                                                                                                                                           |
| Bandwidth                      | 1 kHz, typical                                                                                                                                                                                                                                            |
| Input Impedance                | 1 k $\Omega$ , typical                                                                                                                                                                                                                                    |
| <b>External Detector Input</b> |                                                                                                                                                                                                                                                           |
| Description                    | Input from an external, negative polarity diode detector provides ALC for a test port remote from instrument's front panel                                                                                                                                |
| Connector                      | BNC, female                                                                                                                                                                                                                                               |
| Input Sensitivity              | -500 mV yields approximately -3 dBm at detector's input, typical                                                                                                                                                                                          |
| Bandwidth                      | 50 kHz, typical                                                                                                                                                                                                                                           |
| Input Impedance                | 1 k $\Omega$ , nominal                                                                                                                                                                                                                                    |

**Table 20. Analyzer Environment and Dimensions**

| Description                                                                 | Supplemental Information                                                                                           |                    |                    |
|-----------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------|--------------------|--------------------|
| <b>General Environmental</b>                                                |                                                                                                                    |                    |                    |
| RFI/EMI Susceptibility                                                      | Defined by CISPR Pub. 11, Group 1, Class A, and IEC 50082-1                                                        |                    |                    |
| ESD                                                                         | Minimize using static-safe work procedures and an antistatic bench mat                                             |                    |                    |
| Dust                                                                        | Minimize for optimum reliability                                                                                   |                    |                    |
| <b>Operating Environment</b>                                                |                                                                                                                    |                    |                    |
| Temperature                                                                 | 0 °C to +40 °C<br>Instrument powers up, phase locks, and displays no error messages within this temperature range. |                    |                    |
| Error-Corrected Temperature Range                                           | 25°C ± 5°C<br>with less than 1°C deviation from calibration temp.                                                  |                    |                    |
| Humidity                                                                    | 5% to 95% at +40 °C                                                                                                |                    |                    |
| Altitude                                                                    | 0 to 4500 m (14,760 ft.)                                                                                           |                    |                    |
| <b>Non-Operating Storage Environment</b>                                    |                                                                                                                    |                    |                    |
| Temperature                                                                 | -40 °C to +70 °C                                                                                                   |                    |                    |
| Humidity                                                                    | 0% to 90% at +65 °C (non-condensing)                                                                               |                    |                    |
| Altitude                                                                    | 0 to 15,240 m (50,000 ft.)                                                                                         |                    |                    |
| <b>Cabinet Dimensions</b>                                                   |                                                                                                                    |                    |                    |
|                                                                             | <b>Height</b>                                                                                                      | <b>Width</b>       | <b>Depth</b>       |
| Excluding front and rear panel hardware and feet                            | 223 mm<br>8.75 in                                                                                                  | 426 mm<br>16.75 in | 427 mm<br>16.8 in  |
| As shipped - includes front panel connectors, rear panel bumpers, and feet. | 235 mm<br>9.25 in                                                                                                  | 435 mm<br>17.10 in | 470 mm<br>18.5 in  |
| As shipped plus handles                                                     | 235 mm<br>9.25 in                                                                                                  | 458 mm<br>18 in    | 501 mm<br>19.70 in |
| As shipped plus rack-mount flanges                                          | 235 mm<br>9.25 in                                                                                                  | 483 mm<br>19 in    | 470 mm<br>18.5 in  |
| As shipped plus handles and flanges                                         | 235 mm<br>9.25 in                                                                                                  | 483 mm<br>19 in    | 501 mm<br>19.70 in |
| <b>Weight</b>                                                               |                                                                                                                    |                    |                    |
| Net                                                                         | 24 kg (54 lb), nominal                                                                                             |                    |                    |
| Shipping                                                                    | 32 kg (70 lb), nominal                                                                                             |                    |                    |

**Note:** "Misc. Information" specifications are not included in this E8801/2/3A document.

## Measurement Throughput Summary

### Typical Cycle Time for Measurement Completion

#### Cycle Time with Changes in IF Bandwidth

#### Cycle Time with Changes in Number of Points

#### Data Transfer Time

#### Recall and Sweep Speed

**Table 21. Typical Cycle Time<sup>a,b</sup> (ms)**

|                                                       | Number of Points |     |     |      |
|-------------------------------------------------------|------------------|-----|-----|------|
|                                                       | 101              | 201 | 401 | 1601 |
| <b>Start 1.8 GHz, Stop 2 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected,<br>1-port cal                            | 7                | 10  | 16  | 52   |
| 2-Port cal                                            | 27               | 36  | 55  | 164  |
| <b>Start 300 kHz, Stop 3 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected,<br>1-port cal                            | 48               | 54  | 64  | 104  |
| 2-Port cal                                            | 103              | 119 | 145 | 254  |
| <b>Start 300 kHz, Stop 9 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected,<br>1-port cal                            | 51               | 57  | 64  | 103  |
| 2-Port cal                                            | 112              | 124 | 138 | 220  |

a Typical performance.

b Includes sweep time, retrace time and band-crossing time. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S11) measurement..

**Table 22. Cycle Time vs. IF Bandwidth<sup>a</sup>**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 1 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)



| IF Bandwidth (Hz) | Cycle Time (ms) <sup>b</sup> |
|-------------------|------------------------------|
| 40,000            | 8                            |
| 35,000            | 9                            |
| 30,000            | 11                           |
| 20,000            | 13                           |
| 10,000            | 28                           |
| 7000              | 36                           |
| 5000              | 48                           |
| 3000              | 72                           |
| 1000              | 196                          |
| 300               | 620                          |
| 100               | 1875                         |
| 30                | 8062                         |
| 10                | 17877                        |

**a** Typical performance.

**b** Cycle time includes sweep and retrace time.

### Table 23. Cycle Time vs. Number of Points<sup>a</sup>

Applies to the Preset condition (35 kHz IF bandwidth, correction off) except for the following changes:

- CF = 1 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Number of Points | Cycle Time (ms) <sup>b</sup> |
|------------------|------------------------------|
| 3                | 4                            |
| 11               | 4                            |
| 51               | 5                            |
| 101              | 6                            |
| 201              | 9                            |
| 401              | 16                           |
| 801              | 29                           |
| 1601             | 52                           |

**a** Typical performance.

**b** Cycle time includes sweep and retrace time.

### Table 24. Data Transfer Time<sup>a</sup> (ms)

|                                                                                   | Number of Points |     |     |      |
|-----------------------------------------------------------------------------------|------------------|-----|-----|------|
|                                                                                   | 51               | 201 | 401 | 1601 |
| <b>SCPI over GPIB<br/>(program executed on external PC)<sup>b</sup></b>           |                  |     |     |      |
| 32-bit floating point                                                             | 3                | 7   | 12  | 43   |
| 64-bit floating point                                                             | 4                | 12  | 22  | 84   |
| ASCII                                                                             | 7                | 64  | 24  | 489  |
| <b>SCPI over 100 Mbit/s LAN<br/>(program executed on external PC)<sup>b</sup></b> |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 1   | 1    |
| 64-bit floating point                                                             | 1                | 1   | 1   | 2    |
| ASCII                                                                             | 5                | 15  | 26  | 96   |
| <b>SCPI (program executed in the analyzer)<sup>d</sup></b>                        |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 2   | 3    |
| 64-bit floating point                                                             | 1                | 2   | 2   | 4    |
| ASCII                                                                             | 8                | 29  | 56  | 222  |
| <b>COM (program executed in the analyzer)<sup>e</sup></b>                         |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 1   | 1    |
| Variant type                                                                      | 1                | 1   | 2   | 6    |
| <b>DCOM over 100 Mbit/s LAN<br/>(program executed on external PC)<sup>f</sup></b> |                  |     |     |      |
| 32-bit floating point <sup>g</sup>                                                | 1                | 1   | 1   | 2    |
| Variant type <sup>h</sup>                                                         | 1                | 3   | 6   | 19   |

**a** Typical performance of unit with 500 MHz Pentium III processor.

**b** Measured using a VEE 5.0 program running on a 600 MHz HP Kayak, National Instruments™ GPIB card. Transferred complex S11 data, using "CALC:DATA?SDATA".

**c** Measured using a VEE 5.0 program running on a 600 MHz HP Kayak. Transferred complex S11 data, using "CALC:DATA?SDATA". Speed dependent on LAN traffic, if connected to network.

**d** Measured using a VEE 5.0 program running inside PNA Series Analyzer. Transferred complex S11 data, using "CALC:DATA?SDATA".

**e** Measured using a Visual Basic 6.0 program running inside PNA Series Analyzer. Transferred complex S11 data.

**f** Measured using a Visual Basic 6.0 program running on a 600 MHz HP Kayak. Transferred complex S11 data. Speed dependent on LAN traffic, if connected to network.

**g** Used IArray Transfer.getComplex method for 32-bit floating point.


**h** Used meas.getData method for Variant data type.

**Table 25. Recall and Sweep Speed<sup>a</sup>**


| <b>Operations</b> | <b>Number of Window(s)</b> | <b>Number of Trace(s)</b> | <b>Recall Time (ms)</b> |
|-------------------|----------------------------|---------------------------|-------------------------|
| Recall            | 1                          | 1                         | 49                      |
| Recall and Sweep  | 1                          | 1                         | 59                      |
|                   |                            |                           |                         |
| Recall            | 1                          | 2                         | 82                      |
| Recall and Sweep  | 1                          | 2                         | 96                      |
|                   |                            |                           |                         |
| Recall            | 1                          | 4                         | 159                     |
| Recall and Sweep  | 1                          | 4                         | 203                     |
|                   |                            |                           |                         |
| Recall            | 2                          | 2                         | 93                      |
| Recall and Sweep  | 2                          | 2                         | 115                     |
|                   |                            |                           |                         |
| Recall            | 3                          | 4                         | 158                     |
| Recall and Sweep  | 3                          | 4                         | 218                     |
|                   |                            |                           |                         |
| Recall            | 4                          | 4                         | 187                     |
| Recall and Sweep  | 4                          | 4                         | 247                     |
|                   |                            |                           |                         |
| Recall            | 4                          | 8                         | 340                     |
| Recall and Sweep  | 4                          | 8                         | 507                     |

a CF=177 MHz, Span=200 MHz, 201 points, 35 kHz IF BW

**E8801A, E8802A, and E8803A – Simplified Test Set Block Diagram**

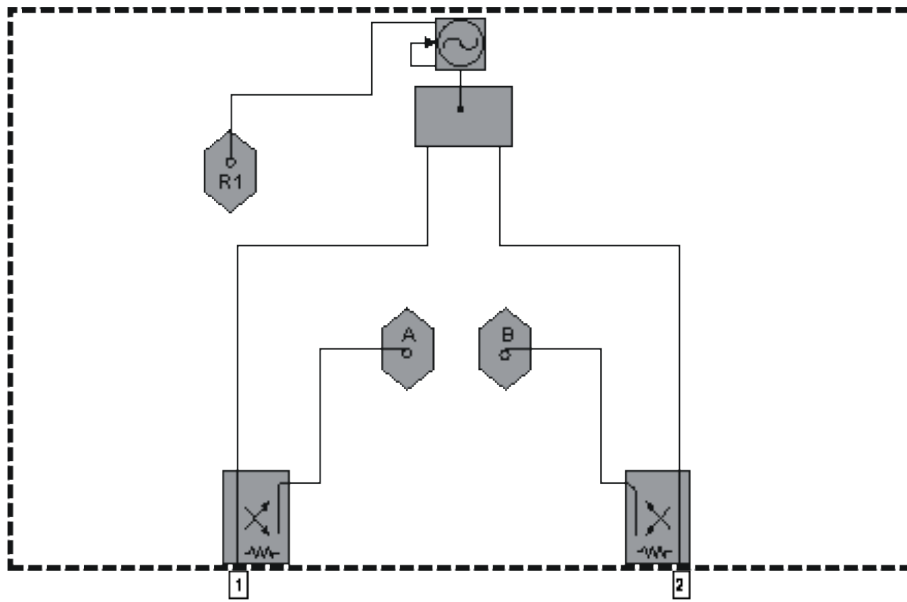

**E8801A, E8802A, and E8803A with Option 014 – Simplified Test Set Block Diagram**

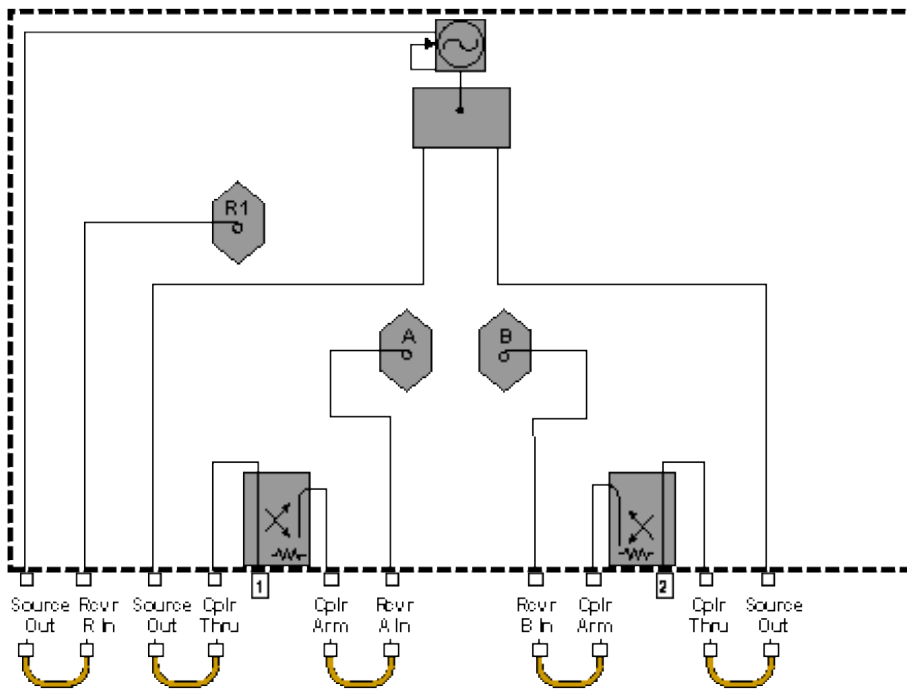

# Technical Specifications for the N3381A, N3382A, N3383A

(Rev. 2004-04-23)

This is a complete list of the N3381A, N3382A, and N3383A network analyzer technical specifications.

- To optimize viewing of uncertainty curves, click the Maximize button.
- To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "N338xA Specifications"
- The uncertainty curves contained in this document apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the [equations](#) used to generate the uncertainty curves.

---

## Definitions

### Corrected System Performance

#### System Dynamic Range

#### Type-N Connectors

#### 3.5 mm Connectors

#### 7-16 Connectors

### Uncorrected Instrument Performance

#### Test Port Output Characteristics (Source)

#### Test Port and Receiver Input Characteristics

### General Information

#### Front-panel Jumper Specs (Option 014 only)

#### Measurement Throughput Summary

#### Test Set Block Diagram

#### Test Set with Option 015 Block Diagram

[See Specs for other PNA models](#)

## Definitions

All specifications and characteristics apply over a 25 °C ±5 °C range (unless otherwise stated) and 90 minutes after the instrument has been turned on.

**Specification (spec.):** Warranted performance. Specifications include guardbands to account for the expected statistical performance distribution, measurement uncertainties, and changes in performance due to environmental

conditions.

**Characteristic (char.):** A performance parameter that the product is expected to meet before it leaves the factory, but that is not verified in the field and is not covered by the product warranty. A characteristic includes the same guardbands as a specification.

**Typical (typ.):** Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Nominal (nom.):** A general, descriptive term that does not imply a level of performance. It is not covered by the product warranty.

**Calibration:** The process of measuring known standards to characterize a network analyzer's systematic (repeatable) errors.

**Corrected (residual):** Indicates performance after error correction (calibration). It is determined by the quality of calibration standards and how well "known" they are, plus system repeatability, stability, and noise.

**Uncorrected (raw):** Indicates instrument performance without error correction. The uncorrected performance affects the stability of a calibration.

**Standard:** When referring to the analyzer, this includes no options unless noted otherwise.

---

## Corrected System Performance

The specifications in this section apply for measurements made with the N3381A, N3382A, and N3383A analyzer with the following conditions:

- 10 Hz IF bandwidth
- No averaging applied to data
- Environmental temperature of 25 °C ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted

---

**Note:** The uncertainty curves contained in these specifications apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the equations used to generate the uncertainty curves.

---

### System Dynamic Range

#### Type-N Connectors

#### 3.5 mm Connectors

#### 7/16 Connectors

## Table 1. System Dynamic Range

| Description                                          | Specification (dB) | Characteristic (dB) |
|------------------------------------------------------|--------------------|---------------------|
| <b>Dynamic range<sup>a</sup> (at test port)</b>      |                    |                     |
| 300 kHz to 25 MHz <sup>b</sup>                       | 125                |                     |
| 25 MHz to 3 GHz <sup>b</sup>                         | 128                |                     |
| 3 GHz to 6 GHz                                       | 118                |                     |
| 6 GHz to 9 GHz                                       | 115                |                     |
| <b>Dynamic range<sup>c</sup> (at receiver input)</b> |                    |                     |
| 300 kHz to 25 MHz <sup>d</sup>                       |                    | 140                 |
| 25 MHz to 3 GHz <sup>d</sup>                         |                    | 143                 |
| 3 GHz to 6 GHz                                       |                    | 133                 |
| 6 GHz to 9 GHz                                       |                    | 130                 |

**a** The test port dynamic range is calculated as the difference between the test port rms noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account.

**b** May be limited to 100 dB at particular frequencies below 750 MHz due to spurious receiver residuals.

**c** The receiver input dynamic range is calculated as the difference between the receiver rms noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its damage level. When the analyzer is in segment sweep mode, frequency segments can be defined with a higher power level when the extended dynamic range is required (i.e. the portion of the device's response with high insertion loss), and reduced power when receiver damage may occur (i.e. the portion of the device's response with low insertion loss). Specification applies only when power is sourced from Port 1. If power is sourced from either Port 2 or Port 3, dynamic range decreases by 3 dB.

**d** May be limited to 115 dB at particular frequencies below 750 MHz due to spurious receiver residuals.

---

**Note:** Receiver Dynamic Range specifications are not included in this N3381/2/3A document.

---

**Note:** This document provides technical specifications for the following calibration kits only: 85032F, 85092C, 85033E, 85093C and 85038A.

---

## Corrected System Performance with Type-N Connectors

### 85032F Calibration Kit

### 85092C Electronic Calibration Module

## Table 2. Corrected System Performance With Type-N Device Connectors, 85032F Calibration Kit


Applies to the N3381A, N3382A, and N3383A analyzer, 85032F (Type-N, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |             |             |
|-----------------------|--------------------|------------------|-------------|-------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz  | 6 to 9 GHz  |
| Directivity           | 49                 | 46               | 40          | 38          |
| Source Match          | 41                 | 40               | 36          | 35          |
| Load Match            | 49                 | 45               | 39          | 37          |
| Reflection Tracking   | $\pm 0.011$        | $\pm 0.021$      | $\pm 0.032$ | $\pm 0.054$ |
| Transmission Tracking | $\pm 0.012$        | $\pm 0.020$      | $\pm 0.055$ | $\pm 0.083$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

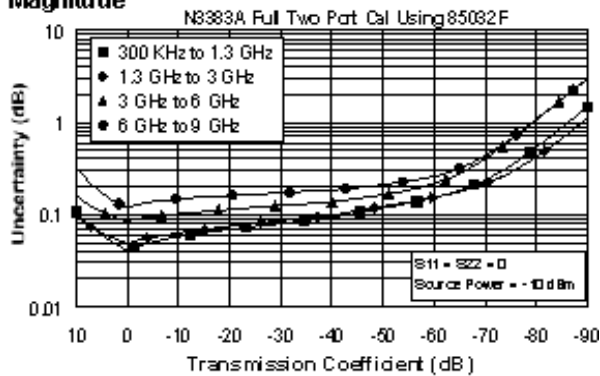


#### Phase

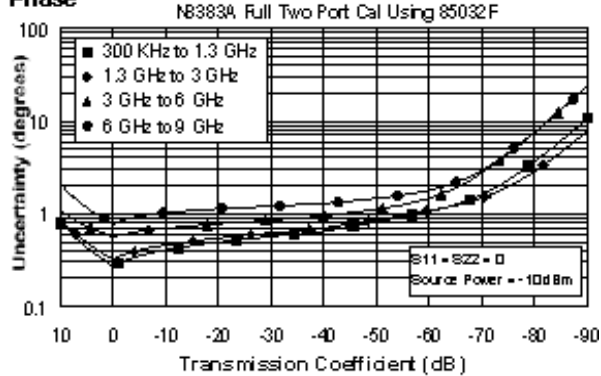


### Reflection Uncertainty (Specifications)

#### Magnitude

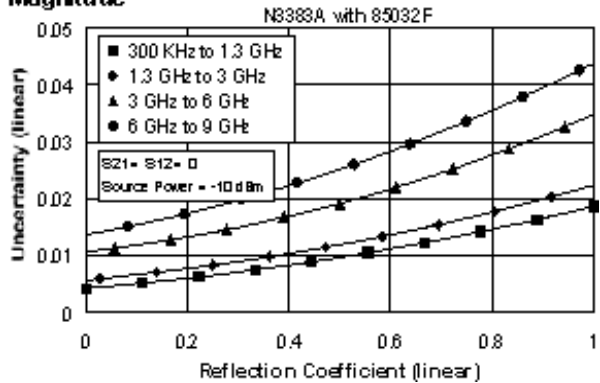

#### Phase

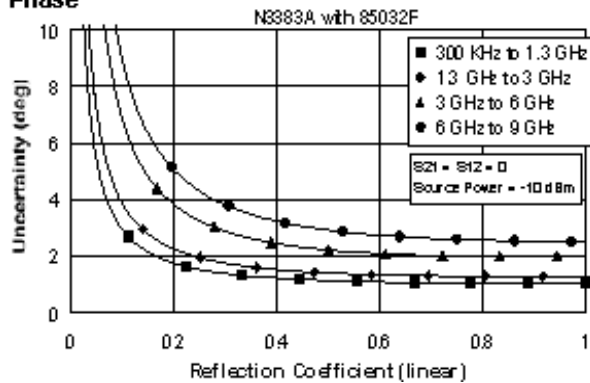

**Table 3. Corrected System Performance With Type-N Device Connectors, 85092C Electronic Calibration Module**

Applies to the N3381A, N3382A, and N3383A analyzer, 85092C (Type-N, 50Ω) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:


- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted




| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 54               | 52         | 47                      |
| Source Match          | 45                 | 44               | 41         | 36                      |
| Load Match            | 47                 | 47               | 44         | 39                      |
| Reflection Tracking   | ±0.040             | ±0.040           | ±0.060     | ±0.070                  |
| Transmission Tracking | ±0.039             | ±0.039           | ±0.068     | ±0.136                  |

### Transmission Uncertainty (Specifications)

#### Magnitude

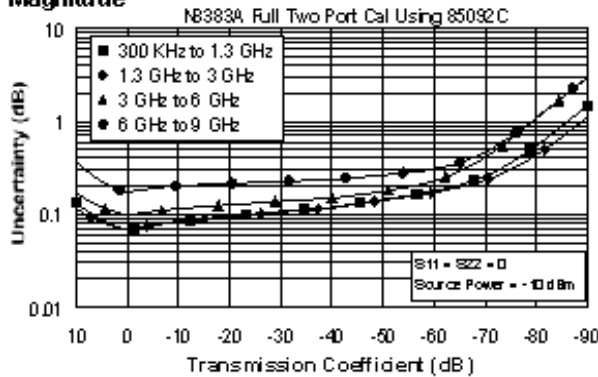


#### Phase

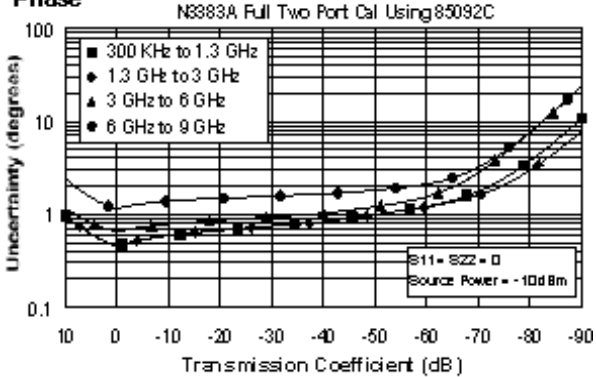


### Reflection Uncertainty (Specifications)

#### Magnitude

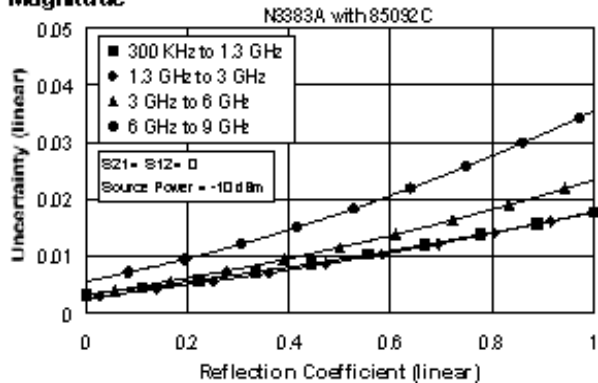

#### Phase

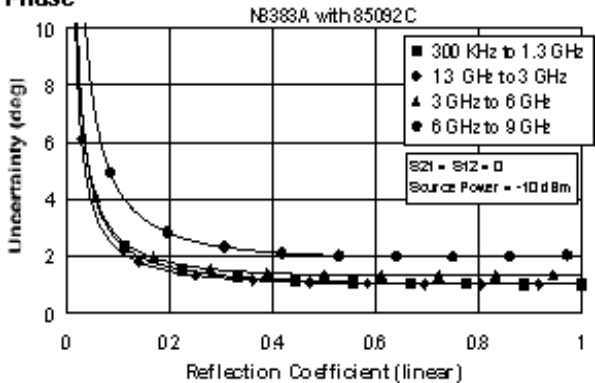

### Corrected System Performance with 3.5 mm Connectors

[85033E Calibration Kit](#)

[85093C Electronic Calibration Module](#)

**Table 4. Corrected System Performance With 3.5 mm Device Connector Type, 85033E Calibration Kit**

Applies to the N3381A, N3382A, and N3383A analyzer, 85033E (3.5 mm, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:


- IF bandwidth = 10 Hz

- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |            |
|-----------------------|--------------------|------------------|------------|------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz |
| Directivity           | 46                 | 44               | 38         | 38         |
| Source Match          | 43                 | 40               | 37         | 36         |
| Load Match            | 46                 | 44               | 38         | 38         |
| Reflection Tracking   | ±0.006             | ±0.007           | ±0.009     | ±0.010     |
| Transmission Tracking | ±0.012             | ±0.021           | ±0.057     | ±0.075     |

### Transmission Uncertainty (Specifications)

#### Magnitude

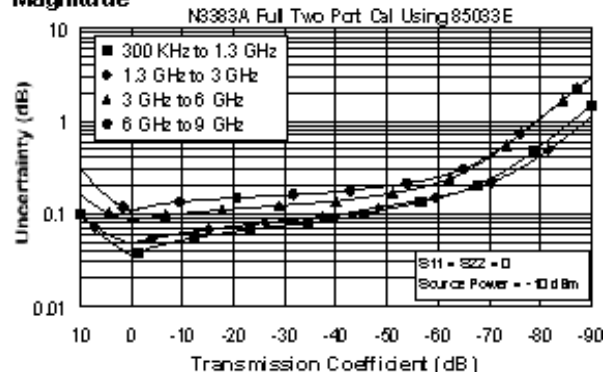


#### Phase

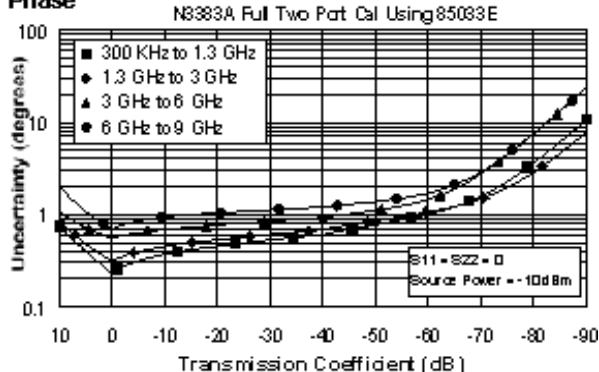


### Reflection Uncertainty (Specifications)

#### Magnitude

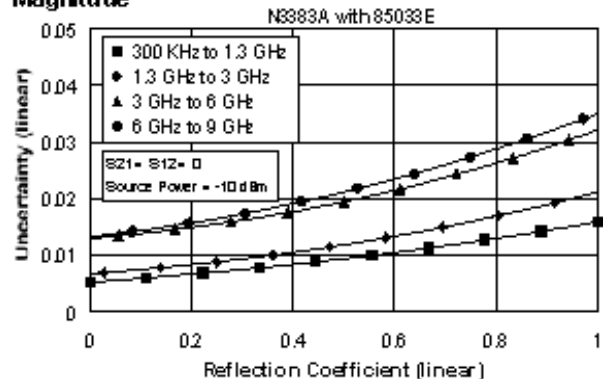

#### Magnitude

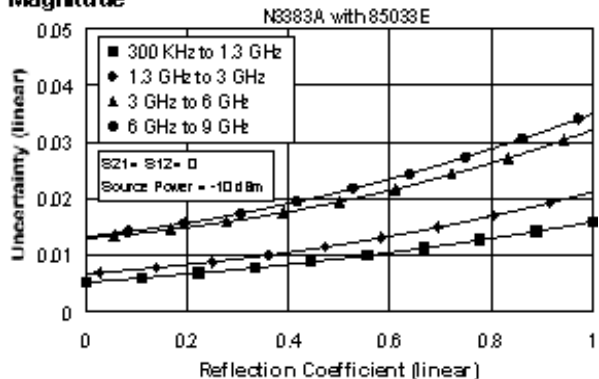

**Table 5. Corrected System Performance With 3.5 mm Device Connector Type, 85093C Electronic Calibration Module**

Applies to the N3381A, N3382A, and N3383A analyzer, 85093C (3.5 mm, 50Ω) electronic calibration (ECal) module, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:


- IF bandwidth = 10 Hz
- No averaging applied to data

- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 52                 | 52               | 51         | 47                      |
| Source Match          | 44                 | 44               | 39         | 34                      |
| Load Match            | 47                 | 47               | 44         | 40                      |
| Reflection Tracking   | ±0.030             | ±0.040           | ±0.050     | ±0.070                  |
| Transmission Tracking | ±0.039             | ±0.049           | ±0.068     | ±0.117                  |

### Transmission Uncertainty (Specifications)

#### Magnitude

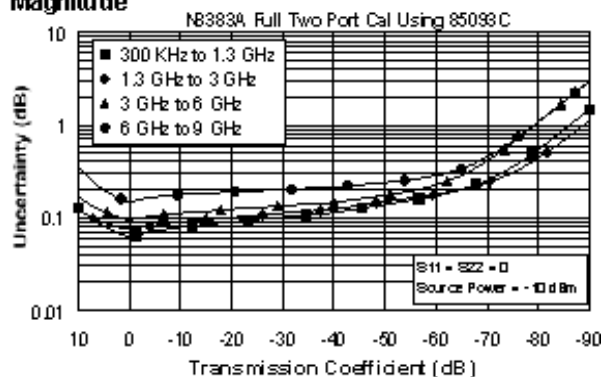


#### Phase

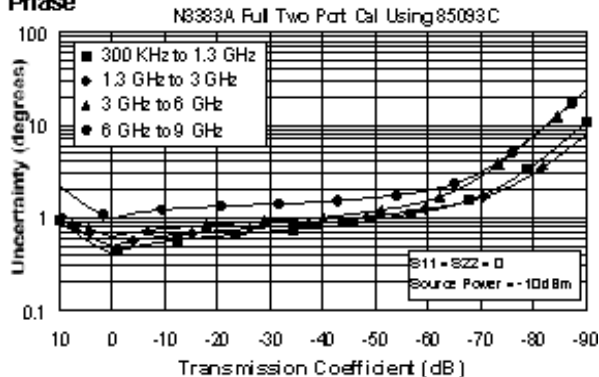


### Reflection Uncertainty (Specifications)

#### Magnitude

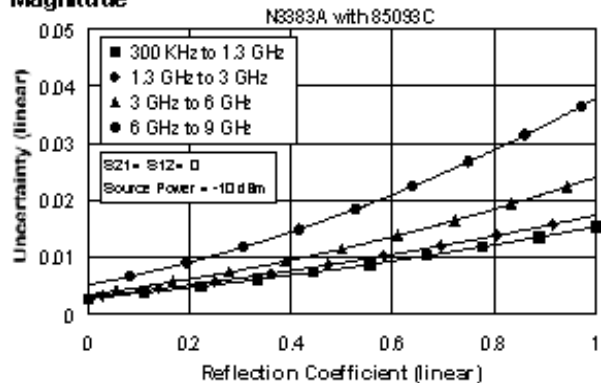

#### Phase

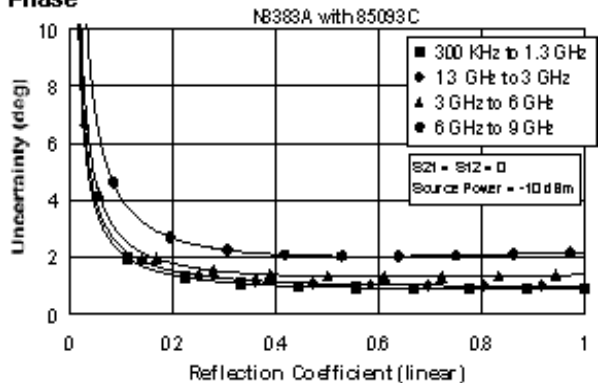

**Table 6. Corrected System Performance With 7-16 Device Connector Type, 85038A Calibration Kit**


Applies to the N3381A, N3382A, and N3383A analyzer, 85038A (7-16, 50Ω) calibration kit, N6314A test port cable, and a full 2-port calibration. Also applies to the following conditions:

- IF bandwidth = 10 Hz
- No averaging applied to data
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature
- Isolation calibration not omitted


| Description           | Specification (dB) |                  |            |                         |
|-----------------------|--------------------|------------------|------------|-------------------------|
|                       | 300 kHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 to 6 GHz | 6 to 9 GHz <sup>a</sup> |
| Directivity           | 40                 | 40               | 36         | 36                      |
| Source Match          | 37                 | 37               | 34         | 34                      |
| Load Match            | 39                 | 39               | 35         | 35                      |
| Reflection Tracking   | ±0.089             | ±0.089           | ±0.115     | ±0.115                  |
| Transmission Tracking | ±0.024             | ±0.033           | ±0.082     | ±0.103                  |

### Transmission Uncertainty (Specifications)

#### Magnitude

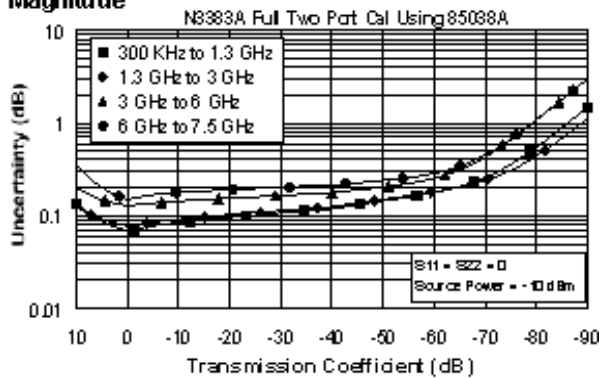


#### Phase

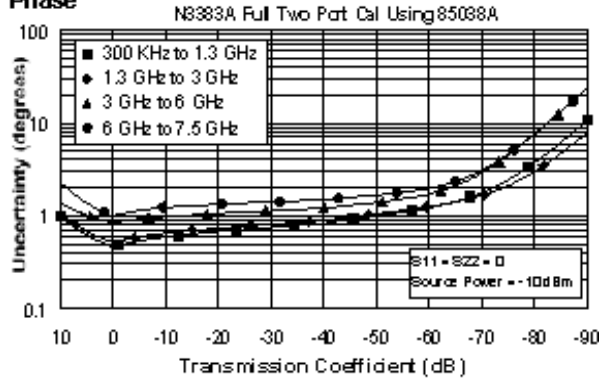

### Reflection Uncertainty (Specifications)

#### Magnitude

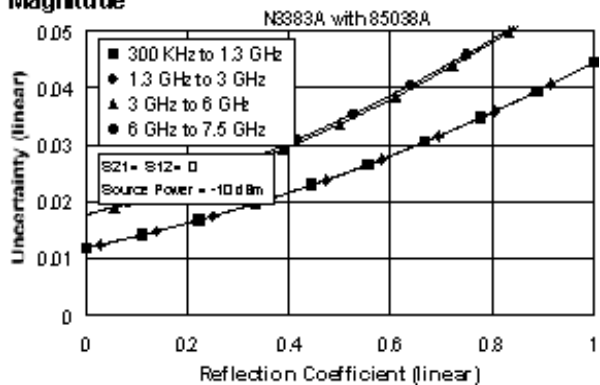

#### Phase

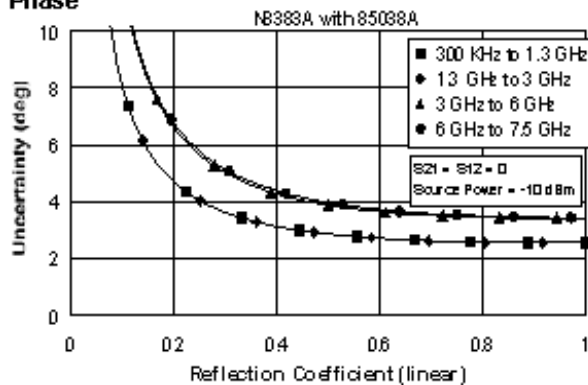


Table 7. Uncorrected Instrument Performance

| Description                | Specification (dB) |                 |                  |                |                |
|----------------------------|--------------------|-----------------|------------------|----------------|----------------|
|                            | 300 kHz to 1 MHz   | 1MHz to 1.3 GHz | 1.3 GHz to 3 GHz | 3 GHz to 6 GHz | 6 GHz to 9 GHz |
| Directivity                | 30                 | 33              | 27               | 20             | 13             |
| Source Match Ports 1 and 2 | 18                 | 18              | 17               | 14             | 12             |
| Source Match Port 3 only   | 18                 | 18              | 17               | 14             | 12             |
| Load Match Ports 1 and 2   | 20                 | 20              | 17               | 13.5           | 11.5           |
| Load Match Port 3 only     | 20                 | 20              | 17               | 13.5           | 11.5           |
| Reflection Tracking        | ±1.5               | ±1.5            | ±1.5             | ±2.5           | ±3.0           |
| Transmission Tracking      | ±1.5               | ±1.5            | ±1.5             | ±2.5           | ±3.0           |

### Test Port Output Characteristics (Source)

Output Frequency

Output Power

Output Signal Purity

**Table 8. Test Port Output Frequency**

| Description                          | Specification      | Supplemental Information                                 |
|--------------------------------------|--------------------|----------------------------------------------------------|
| <b>Range:</b>                        |                    |                                                          |
| N3381A                               | 300 kHz to 3.0 GHz |                                                          |
| N3382A                               | 300 kHz to 6.0 GHz |                                                          |
| N3383A                               | 300 kHz to 9.0 GHz |                                                          |
| <b>Resolution</b>                    | 1 Hz               |                                                          |
| <b>Source Stability</b>              |                    | ±1 ppm, 0° to 40 °C, typical<br>±1ppm/year maximum       |
| <b>Source Stability (Option 1E5)</b> |                    | ±0.05 ppm, 0° to 40 °C, typical<br>±0.1 ppm/year maximum |
| <b>CW Accuracy</b>                   | ±3 ppm             |                                                          |

|                                    |        |  |
|------------------------------------|--------|--|
| <b>CW Accuracy</b><br>(Option 1E5) | ±1 ppm |  |
|------------------------------------|--------|--|

**Table 9. Test Port Output Power<sup>a</sup>**

| Description                              | Specification  | Supplemental Information                                                               |
|------------------------------------------|----------------|----------------------------------------------------------------------------------------|
| <b>Level Accuracy</b>                    |                |                                                                                        |
|                                          |                | Variation from 0 dBm in power range 0 (step attenuator at 0 dB)<br>±1.5dB below 10 MHz |
| 300 kHz to 6 GHz                         | ±1.0 dB        |                                                                                        |
| 6 GHz to 9 GHz                           | ±2.0 dB        |                                                                                        |
| <b>Level Linearity</b>                   |                |                                                                                        |
|                                          |                | Variation from 0 dBm in power range 0                                                  |
| 300 kHz to 9 GHz                         | ±0.3 dB        | -15 to +5 dBm                                                                          |
| 300 kHz to 1 MHz                         | ±1.0 dB        | +5 to +10 dBm                                                                          |
| 1 MHz to 6 GHz                           | ±0.5 dB        | +5 to +10 dBm                                                                          |
| 6 GHz to 9 GHz                           | ±0.5 dB        | +5 to +7 dBm                                                                           |
| <b>Range<sup>b</sup></b>                 |                |                                                                                        |
| 300 kHz to 6 GHz                         | -15 to +10 dBm |                                                                                        |
| 6 GHz to 9 GHz                           | -15 to +7 dBm  |                                                                                        |
| <b>Range<sup>b</sup></b><br>(Option 1E1) |                |                                                                                        |
| 300 kHz to 6 GHz                         | -85 to +10 dBm |                                                                                        |
| 6 GHz to 9 GHz                           | -85 to +7 dBm  |                                                                                        |
| <b>Sweep Range</b>                       |                |                                                                                        |
| Port 1:                                  |                |                                                                                        |
| 300 kHz to 6 GHz                         | 25 dB          |                                                                                        |
| 6 GHz to 9 GHz                           | 22 dB          |                                                                                        |
| <b>Level Resolution</b>                  | 0.01 dB        |                                                                                        |

<sup>a</sup> Source output performance on port 1 only. Port 2 and port 3 output performance is typically 3 dB less.

<sup>b</sup> Power to which the source can be set and phase lock is assured.

**Table 10. Test Port Output Signal Purity**

| Description                           | Specification | Supplemental Information               |
|---------------------------------------|---------------|----------------------------------------|
| <b>Harmonics (2nd or 3rd)</b>         |               |                                        |
| at max output power (< 25 MHz)        |               | < -25 dBc, typical                     |
| at max output power (25 MHz to 9 GHz) |               | < -25 dBc, characteristic <sup>a</sup> |
| at 0 dBm output                       |               | < -35 dBc, typical                     |
| at -10 dBm output                     |               | < -38 dBc, typical, in power range 0   |
| <b>Non-harmonic Spurious</b>          |               |                                        |
| at max output                         |               | -30 dBc, typical for offset freq>1kHz  |
| at -10 dBm output                     |               | -50 dBc, typical for offset freq >1kHz |

<sup>a</sup> Typical below 25 MHz.

**Test Port and Receiver Input Characteristics**

**Input Levels**

**Trace Noise**

**Reference Level and Stability**

**Dynamic Accuracy**

**Group Delay**

**Table 11. Test Port and Receiver Input Levels**

| Description                          | Specification | Supplemental Information |
|--------------------------------------|---------------|--------------------------|
| <b>Maximum Test Port Input Level</b> |               |                          |
| 300 kHz to 25 MHz                    | +10 dBm       | <0.6 dB compression      |
| 25 MHz to 3 GHz                      | +10 dBm       | <0.4 dB compression      |
| 3 GHz to 6 GHz                       | +10 dBm       | <0.7 dB compression      |
| 6 GHz to 9 GHz                       | +7 dBm        | <0.7 dB compression      |
| <b>Damage Level</b>                  |               |                          |
| Test Port 1, 2, 3                    |               | +30 dBm or ±30 VDC, typ. |
| R, A, B, C (Opt. 014)                |               | +15 dBm or ±5 VDC, typ.  |
| Coupler Thru (Opt. 014)              |               | +33 dBm or ±0 VDC, typ.  |

| <b>Test Port Noise Floor<sup>a</sup></b> |                               |  |
|------------------------------------------|-------------------------------|--|
| 300 kHz to 25 MHz <sup>b</sup>           |                               |  |
| 10 Hz IF Bandwidth                       | = -115 dBm                    |  |
| 1 kHz IF Bandwidth                       | = -95 dBm                     |  |
| 25 MHz to 3 GHz <sup>b</sup>             |                               |  |
| 10 Hz IF Bandwidth                       | = -118 dBm                    |  |
| 1 kHz IF Bandwidth                       | = -98 dBm                     |  |
| 3 GHz to 9 GHz                           |                               |  |
| 10 Hz IF Bandwidth                       | ≤ -108 dBm                    |  |
| 1 kHz IF Bandwidth                       | ≤ -88 dBm                     |  |
| <b>Receiver Noise Floor<sup>a</sup></b>  |                               |  |
| 300 kHz to 25 MHz <sup>c</sup>           |                               |  |
| 10 Hz IF Bandwidth                       | ≤ -130 dBm,<br>characteristic |  |
| 1 kHz IF Bandwidth                       | ≤ -110 dBm,<br>characteristic |  |
| 25 MHz to 3 GHz <sup>c</sup>             |                               |  |
| 10 Hz IF Bandwidth                       | = -133 dBm,<br>characteristic |  |
| 1 kHz IF Bandwidth                       | = -113 dBm,<br>characteristic |  |
| 6 GHz to 9 GHz                           |                               |  |
| 10 Hz IF Bandwidth                       | ≤ -123 dBm,<br>characteristic |  |
| 1 kHz IF Bandwidth                       | ≤ -103 dBm,<br>characteristic |  |
| <b>Crosstalk</b>                         |                               |  |
| (S <sub>21</sub> , S <sub>31</sub> ):    |                               |  |
| 300 kHz to 1 MHz                         | <-120 dB                      |  |
| 1 MHz to 25 MHz                          | <-125 dB                      |  |
| 25 MHz to 3 GHz                          | <-126 dB                      |  |
| 3 GHz to 6 GHz                           | <-117 dB                      |  |



|                                                  |          |                         |
|--------------------------------------------------|----------|-------------------------|
| 6 GHz to 9 GHz                                   | <-106 dB |                         |
| <b>(S12, S13):</b>                               |          |                         |
| 300 kHz to 1 MHz                                 | <-120 dB |                         |
| 1 MHz to 25 MHz                                  | <-125 dB |                         |
| 25 MHz to 3 GHz                                  | <-126 dB |                         |
| 3 GHz to 6 GHz                                   | <-113 dB |                         |
| 6 GHz to 9 GHz                                   | <-106 dB |                         |
| <b>(S23, S32):</b>                               |          |                         |
| 300 kHz to 1 MHz                                 | <-120 dB |                         |
| 1 MHz to 3 GHz                                   | <-125 dB |                         |
| 3 GHz to 6 GHz                                   | <-115 dB |                         |
| 6 GHz to 9 GHz                                   | <-107 dB |                         |
| <b>Maximum Receiver Input Level (A, B, R, C)</b> |          |                         |
| 300 kHz to 6 GHz                                 |          | dBm, typical            |
| 6 GHz to 9 GHz                                   |          | dBm, typical            |
| <b>Reference Input Level (R)<sup>d</sup></b>     |          |                         |
| 300 kHz to 9 GHz                                 |          | -10 to -35 dBm, typical |
| <b>Maximum Coupler Input Level (Opt 014)</b>     |          |                         |
| 300 kHz to 9 GHz                                 |          | +33 dBm, typical        |

<sup>a</sup> Total average (RMS) noise power calculated as the mean value of a linear magnitude trace expressed in dBm.

<sup>b</sup> May be limited to -90 dBm at particular frequencies below 750 MHz due to spurious receiver residuals.

<sup>c</sup> May be limited to -105 dBm at particular frequencies below 750 MHz due to spurious receiver residuals.

<sup>d</sup> Input level to maintain phase lock.

**Table 12. Test Port Input (Trace Noise)**

| Description                              | Specification  | Supplemental Information |
|------------------------------------------|----------------|--------------------------|
| <b>Trace Noise<sup>a</sup> Magnitude</b> |                |                          |
| 1 kHz IF Bandwidth                       | < 0.002 dB rms |                          |
| 10 kHz IF Bandwidth                      | < 0.005 dB rms |                          |
| <b>Trace Noise<sup>a</sup> Phase</b>     |                |                          |
| 1 kHz IF Bandwidth                       | < 0.010° rms   |                          |
| 10 kHz IF Bandwidth                      | < 0.035° rms   |                          |

<sup>a</sup> Trace noise is defined as a ratio measurement of a through or a full reflection, with the source set to 0 dBm.

**Table 13. Test Port Input (Reference Level and Stability)**

| Description                            | Specification | Supplemental Information |
|----------------------------------------|---------------|--------------------------|
| <b>Reference Level Magnitude</b>       |               |                          |
| Range                                  | ±200 dB       |                          |
| Resolution                             | 0.001 dB      |                          |
| <b>Reference Level Phase</b>           |               |                          |
| Range                                  | ±500°         |                          |
| Resolution                             | 0.01°         |                          |
| <b>Stability Magnitude<sup>a</sup></b> |               |                          |
| 300 kHz to 3 GHz                       |               | 0.02 dB/°C, typical      |
| 3 GHz to 6 GHz                         |               | 0.04 dB/°C, typical      |
| 6 GHz to 9 GHz                         |               | 0.06 dB/°C, typical      |
| <b>Stability Phase<sup>a</sup></b>     |               |                          |
| 300 kHz to 3 GHz                       |               | 0.2°/°C, typical         |
| 3 GHz to 6 GHz                         |               | 0.3°/°C, typical         |
| 6 GHz to 9 GHz                         |               | 0.6°/°C, typical         |

<sup>a</sup> Stability is defined as a ratio measurement at the test port.


**Table 14. Test Port Input (Dynamic Accuracy specification<sup>a</sup>)**

Accuracy of the test port input power reading is relative to the reference input power level. Applies to input ports 1 and 2 with the following conditions:

- IF bandwidth = 10 Hz
- Environmental temperature 25° ±5 °C, with < 1 °C deviation from calibration temperature


300 kHz to 3 GHz

**Magnitude**

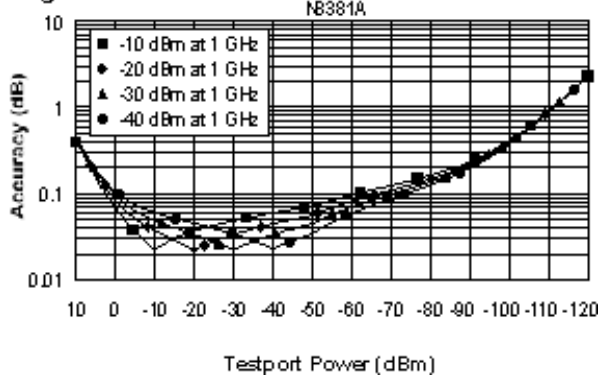

300 kHz to 3 GHz


**Phase**

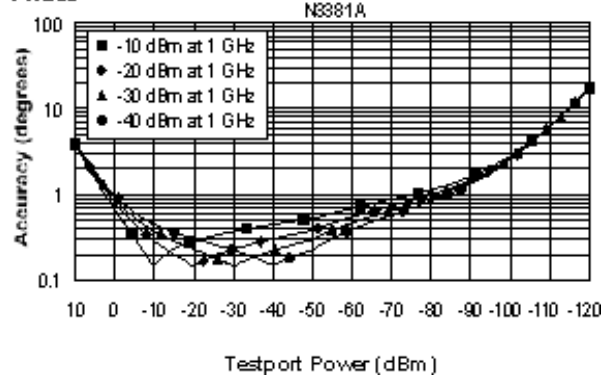


300 kHz to 6 GHz

300 kHz to 6 GHz

**Magnitude**

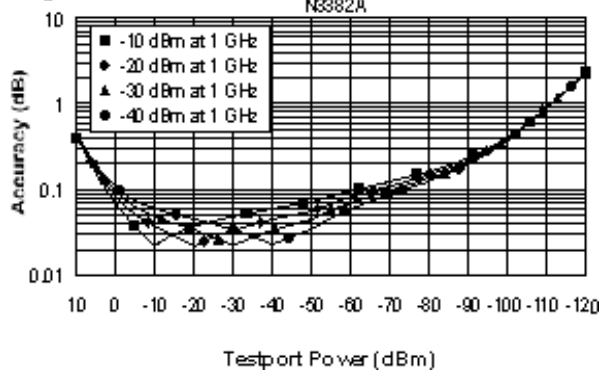


**Phase**

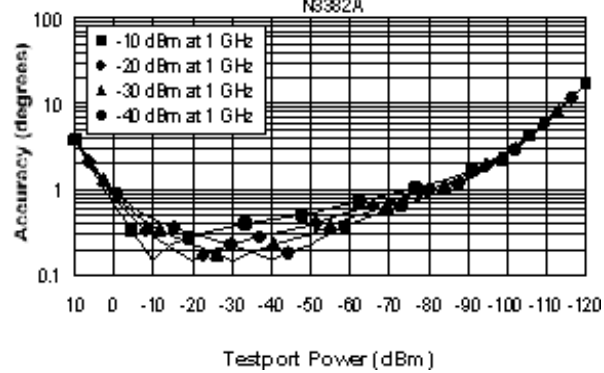


300 kHz to 9 GHz

300 kHz to 9 GHz

**Magnitude**

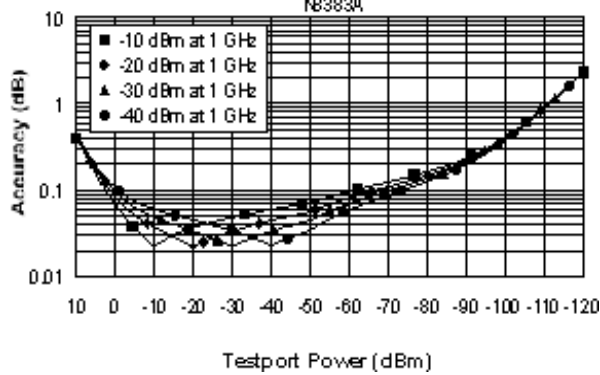

**Phase**

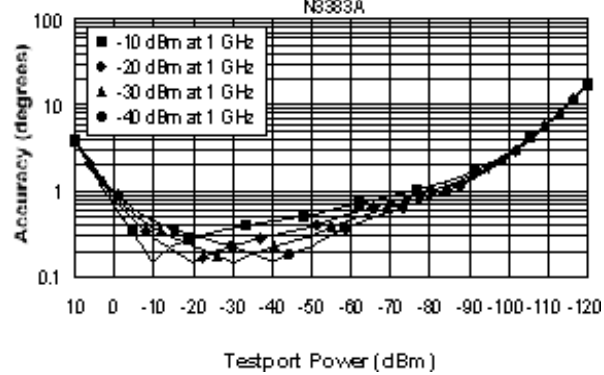


aDynamic accuracy is verified with the following measurements:

- compression over frequency
- IF linearity at a single frequency of 1.195 GHz and a reference level of -20 dBm

**Table 15. Test Port Input (Group Delay)<sup>a</sup>**

| Description           | Specification                          | Supplemental Information                                                             |
|-----------------------|----------------------------------------|--------------------------------------------------------------------------------------|
| Aperture (selectable) | (frequency span)/(number of points -1) |                                                                                      |
| Maximum Aperture      | 20% of frequency span                  |                                                                                      |
| Range                 | 0.5 x (1/minimum aperture)             |                                                                                      |
| Maximum Delay         |                                        | Limited to measuring no more than 180° of phase change within the minimum aperture.) |
| Accuracy              |                                        | See graph below. Char.                                                               |

The following graph shows group delay accuracy with type-N full 2-port calibration and a 10 Hz IF bandwidth. Insertion loss is assumed to be < 2 dB and electrical length to be ten meters.

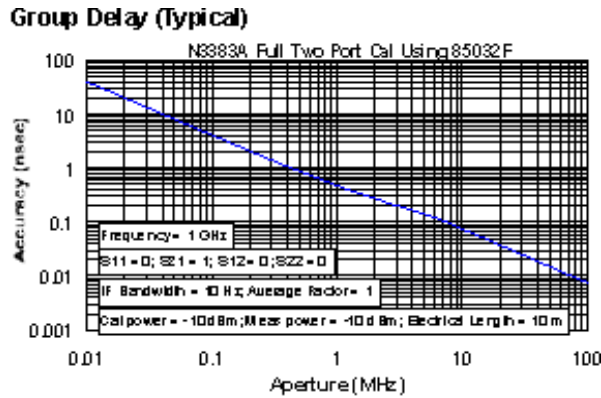

In general, the following formula can be used to determine the accuracy, in seconds, of specific group delay measurement:

$$\pm \text{Phase Accuracy (deg)} / [360 \times \text{Aperture (Hz)}]$$

Depending on the aperture and device length, the phase accuracy used is either incremental phase accuracy or worst case phase accuracy.

a Group delay is computed by measuring the phase change within a specified frequency step (determined by the frequency span and the number of points per sweep).

## General Information

### [System Bandwidths](#)

### [Front Panel](#)

### [Rear Panel](#)

### [Environment and Dimensions](#)

**Table 16. System Bandwidths**

| Description                  | Specification | Supplemental Information                                                            |
|------------------------------|---------------|-------------------------------------------------------------------------------------|
| <b>IF Bandwidth Settings</b> |               |                                                                                     |
| Range                        |               | 1 Hz to 40 kHz in a 1, 2, 3, 5, 7, 10 sequence up to 30 kHz, 35 kHz, 40kHz, nominal |

**Table 17. Front Panel Information**

| Description               | Supplemental Information                                                                        |
|---------------------------|-------------------------------------------------------------------------------------------------|
| <b>RF Connectors</b>      |                                                                                                 |
| Type                      | Type-N, female; 50 $\Omega$ , nominal                                                           |
| Center Pin Protrusion     | 0.204 to 0.207 in., characteristic                                                              |
| <b>Probe Power</b>        |                                                                                                 |
| Connector                 | 3-pin connector, male                                                                           |
| Positive Supply           | +15 VDC $\pm$ 2%, 400 mA, max, characteristic                                                   |
| Negative Supply           | -12.6 VDC $\pm$ 5%, 300 mA, max, characteristic                                                 |
| <b>Display</b>            |                                                                                                 |
| Size                      | 21.3 cm (8.4 in) diagonal color active matrix LCD; 640 (horizontal) X 480 (vertical) resolution |
| Refresh Rate              | Vertical 59.83 Hz; Horizontal 31.41 Hz                                                          |
| <b>Display Range</b>      |                                                                                                 |
| Magnitude                 | $\pm$ 200 dB (at 20 dB/div), max                                                                |
| Phase                     | $\pm$ 180°, max                                                                                 |
| Polar                     | 10 pUnits, min<br>1000 Units, max                                                               |
| <b>Display Resolution</b> |                                                                                                 |
| Magnitude                 | 0.001 dB/div, min                                                                               |
| Phase                     | 0.01°/div, min                                                                                  |
| <b>Marker Resolution</b>  |                                                                                                 |
| Magnitude                 | 0.001 dB, min                                                                                   |
| Phase                     | 0.01°, min                                                                                      |
| Polar                     | 0.01 mUnit, min; 0.01°, min                                                                     |

**Table 18. Rear Panel Information**

| Description                | Supplemental Information    |
|----------------------------|-----------------------------|
| <b>10 MHz Reference In</b> |                             |
| Connector                  | BNC, female                 |
| Input Frequency            | 10 MHz $\pm$ 1 ppm, typical |
| Input Level                | -15 dBm to +20 dBm, typical |
| Input <u>Impedance</u>     | 200 $\Omega$ , nom.         |

| <b>10 MHz Reference Out</b> |                                                                                                                                                                                                                    |
|-----------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Connector                   | BNC, female                                                                                                                                                                                                        |
| Output Frequency            | 10 MHz $\pm$ 10 ppm, typical                                                                                                                                                                                       |
| Signal Type                 | Sine Wave, typical                                                                                                                                                                                                 |
| Output Level                | +10 dBm $\pm$ 4 dB into 50 $\Omega$ , typical                                                                                                                                                                      |
| Output Impedance            | 50 $\Omega$ , nominal                                                                                                                                                                                              |
| Harmonics                   | <-40 dBc, typical                                                                                                                                                                                                  |
| <b>VGA Video Output</b>     |                                                                                                                                                                                                                    |
| Connector                   | 15-pin mini D-Sub; Drives VGA compatible monitors                                                                                                                                                                  |
| Devices Supported:          | Resolutions:                                                                                                                                                                                                       |
| Flat Panel (TFT)            | 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                                   |
| Flat Panel (DSTN)           | 800 X 600, 640 X 480                                                                                                                                                                                               |
| CRT Monitor                 | 1280 X 1024, 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                      |
|                             | Simultaneous operation of the internal and external displays is allowed, but with 640 X 480 resolution only. If you change resolution, you can only view the external display (internal display will "white out"). |
| <b>Test Set IO</b>          | 25-pin D-Sub connector, available for external test set control                                                                                                                                                    |
| <b>Aux IO</b>               | 25-pin D-Sub connector, male, analog and digital IO                                                                                                                                                                |
| <b>Handler IO</b>           | 36-pin IDC D-ribbon socket connector; all input/output signals are default set to negative logic; can be reset to positive logic via GPIB command                                                                  |
| <b>GPIB</b>                 | 24-pin D-sub (Type D-24), female; compatible with IEEE-488.                                                                                                                                                        |
| <b>Parallel Port (LPT1)</b> | 25-pin D-Sub connector, female; provides connection to printers or any other parallel port peripherals                                                                                                             |
| <b>Serial Port (COM 1)</b>  | 9-pin D-Sub, male; compatible with RS-232                                                                                                                                                                          |
| <b>USB Port</b>             |                                                                                                                                                                                                                    |
|                             | Universal Serial Bus jack, Type A configuration (4 contacts inline, contact 1 on left); female                                                                                                                     |
| Contact 1                   | Vcc: 4.75 to 5.25 VDC, 500 mA, maximum                                                                                                                                                                             |
| Contact 2                   | -Data                                                                                                                                                                                                              |
| Contact 3                   | +Data                                                                                                                                                                                                              |
| Contact 4                   | Ground                                                                                                                                                                                                             |

|                                  |                                                                                    |
|----------------------------------|------------------------------------------------------------------------------------|
| <b>LAN</b>                       | 10/100BaseT Ethernet, 8-pin configuration; auto selects between the two data rates |
| <b>Line Power<sup>a, b</sup></b> |                                                                                    |
| Frequency at 110/115 V           | 50/60/400 Hz                                                                       |
| Frequency at 230/240 V           | 50/60Hz                                                                            |
| Maximum Watts                    | 350 W                                                                              |

**a** A third-wire ground is required.

**b** Power supply has a voltage autoswitching feature.

**Note:** Option H08 and Option H11 specifications are not provided in this N3381/2/3A specifications document.

**Table 19. Rear Panel Information (continued)**

| Description                    | Supplemental Information                                                                                                                                                                                                                                  |
|--------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>External AM Input</b>       |                                                                                                                                                                                                                                                           |
| Description                    | Input provides low-frequency AM modulation to test port output signal, or shifts the test port output. Zero volts input gives the power level set by the instrument, a positive voltage gives a higher level, and a negative voltage gives a lower level. |
| Connector                      | BNC, female                                                                                                                                                                                                                                               |
| Input Sensitivity              | 8 dB/V, typical                                                                                                                                                                                                                                           |
| Bandwidth                      | 1 kHz, typical                                                                                                                                                                                                                                            |
| Input Impedance                | 1 k $\Omega$ , nominal                                                                                                                                                                                                                                    |
| <b>External Detector Input</b> |                                                                                                                                                                                                                                                           |
| Description                    | Input from an external, negative polarity diode detector provides ALC for a test port remote from instrument's front panel                                                                                                                                |
| Connector                      | BNC, female                                                                                                                                                                                                                                               |
| Input Sensitivity              | -500 mV yields approximately -3 dBm at detector's input, typical                                                                                                                                                                                          |
| Bandwidth                      | 50 kHz, typical                                                                                                                                                                                                                                           |
| Input Impedance                | 1 k $\Omega$ , typical                                                                                                                                                                                                                                    |

**Table 20. Analyzer Environment and Dimensions**

| Description                                                                 | Supplemental Information                                                                                           |                    |                    |
|-----------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------|--------------------|--------------------|
| <b>General Environmental</b>                                                |                                                                                                                    |                    |                    |
| RFI/EMI Susceptibility                                                      | Defined by CISPR Pub. 11, Group 1, Class A, and IEC 50082-1                                                        |                    |                    |
| ESD                                                                         | Minimize using static-safe work procedures and an antistatic bench mat                                             |                    |                    |
| Dust                                                                        | Minimize for optimum reliability                                                                                   |                    |                    |
| <b>Operating Environment</b>                                                |                                                                                                                    |                    |                    |
| Temperature                                                                 | 0 °C to +40 °C<br>Instrument powers up, phase locks, and displays no error messages within this temperature range. |                    |                    |
| Error-Corrected Temperature Range                                           | 25°C ± 5°C<br>with less than 1°C deviation from calibration temp.                                                  |                    |                    |
| Humidity                                                                    | 5% to 95% at +40 °C                                                                                                |                    |                    |
| Altitude                                                                    | 0 to 4500 m (14,760 ft.)                                                                                           |                    |                    |
| <b>Non-Operating Storage Environment</b>                                    |                                                                                                                    |                    |                    |
| Temperature                                                                 | -40 °C to +70 °C                                                                                                   |                    |                    |
| Humidity                                                                    | 0% to 90% at +65 °C (non-condensing)                                                                               |                    |                    |
| Altitude                                                                    | 0 to 15,240 m (50,000 ft.)                                                                                         |                    |                    |
| <b>Cabinet Dimensions</b>                                                   |                                                                                                                    |                    |                    |
|                                                                             | Height                                                                                                             | Width              | Depth              |
| Excluding front and rear panel hardware and feet                            | 223 mm<br>8.75 in                                                                                                  | 426 mm<br>16.75 in | 427 mm<br>16.8 in  |
| As shipped - includes front panel connectors, rear panel bumpers, and feet. | 235 mm<br>9.25 in                                                                                                  | 435 mm<br>17.10 in | 470 mm<br>18.5 in  |
| As shipped plus handles                                                     | 235 mm<br>9.25 in                                                                                                  | 458 mm<br>18 in    | 501 mm<br>19.70 in |
| As shipped plus rack-mount flanges                                          | 235 mm<br>9.25 in                                                                                                  | 483 mm<br>19 in    | 470 mm<br>18.5 in  |
| As shipped plus handles and flanges                                         | 235 mm<br>9.25 in                                                                                                  | 483 mm<br>19 in    | 501 mm<br>19.70 in |
| <b>Weight</b>                                                               |                                                                                                                    |                    |                    |
| Net                                                                         | 24 kg (54 lb), nominal                                                                                             |                    |                    |
| Shipping                                                                    | 32 kg (70 lb), nominal                                                                                             |                    |                    |



**Note:** "Misc. Information" specifications are not included in this N3381/2/3A document.

## Measurement Throughput Summary

### Typical Cycle Time for Measurement Completion

#### Cycle Time with Changes in IF Bandwidth

#### Cycle Time with Changes in Number of Points

#### Data Transfer Time

#### Recall and Sweep Speed

**Table 21. Typical Cycle Time<sup>a,b</sup> (ms)**

|                                                       | Number of Points |     |     |      |
|-------------------------------------------------------|------------------|-----|-----|------|
|                                                       | 101              | 201 | 401 | 1601 |
| <b>Start 1.8 GHz, Stop 2 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected, 1-port cal                               | 8                | 11  | 17  | 53   |
| 2-Port cal                                            | 27               | 36  | 55  | 164  |
| <b>Start 300 kHz, Stop 3 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected, 1-port cal                               | 48               | 54  | 64  | 104  |
| 2-Port cal                                            | 103              | 119 | 145 | 254  |
| <b>Start 300 kHz, Stop 9 GHz, 35 kHz IF bandwidth</b> |                  |     |     |      |
| Uncorrected, 1-port cal                               | 45               | 55  | 61  | 99   |
| 2-Port cal                                            | 99               | 119 | 133 | 212  |

**a** Typical performance.

**b** Includes sweep time, retrace time and band-crossing time. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S11) measurement.

**c** Option 010 only. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S11) measurement.

**Table 22. Cycle Time vs. IF Bandwidth<sup>a</sup>**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 1 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| IF Bandwidth (Hz) | Cycle Time (ms) <sup>b</sup> |
|-------------------|------------------------------|
| 40,000            | 8                            |
| 35,000            | 9                            |
| 30,000            | 11                           |
| 20,000            | 13                           |
| 10,000            | 28                           |
| 7000              | 36                           |
| 5000              | 48                           |
| 3000              | 72                           |
| 1000              | 196                          |
| 300               | 620                          |
| 100               | 1875                         |
| 30                | 8062                         |
| 10                | 17877                        |

**a** Typical performance.

**b** Cycle time includes sweep and retrace time.

### Table 23. Cycle Time vs. Number of Points<sup>a</sup>

Applies to the Preset condition (35 kHz IF bandwidth, correction off) except for the following changes:

- CF = 1 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Number of Points | Cycle Time (ms) <sup>b</sup> |
|------------------|------------------------------|
| 3                | 4                            |
| 11               | 4                            |
| 51               | 5                            |
| 101              | 6                            |
| 201              | 9                            |
| 401              | 16                           |
| 801              | 29                           |
| 1601             | 52                           |

**a** Typical performance.

**b** Cycle time includes sweep and retrace time.

### Table 24. Data Transfer Time<sup>a</sup> (ms)

|                                                                                   | Number of Points |     |     |      |
|-----------------------------------------------------------------------------------|------------------|-----|-----|------|
|                                                                                   | 51               | 201 | 401 | 1601 |
| <b>SCPI over GPIB<br/>(program executed on external PC)<sup>b</sup></b>           |                  |     |     |      |
| 32-bit floating point                                                             | 3                | 7   | 12  | 43   |
| 64-bit floating point                                                             | 4                | 12  | 22  | 84   |
| ASCII                                                                             | 7                | 64  | 124 | 489  |
| <b>SCPI over 100 Mbit/s LAN<br/>(program executed on external PC)<sup>b</sup></b> |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 1   | 1    |
| 64-bit floating point                                                             | 1                | 1   | 1   | 2    |
| ASCII                                                                             | 5                | 15  | 26  | 96   |
| <b>SCPI (program executed in the analyzer)<sup>d</sup></b>                        |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 2   | 3    |
| 64-bit floating point                                                             | 1                | 2   | 2   | 4    |
| ASCII                                                                             | 8                | 29  | 56  | 222  |
| <b>COM (program executed in the analyzer)<sup>e</sup></b>                         |                  |     |     |      |
| 32-bit floating point                                                             | 1                | 1   | 1   | 1    |
| Variant type                                                                      | 1                | 1   | 2   | 6    |
| <b>DCOM over 100 Mbit/s LAN<br/>(program executed on external PC)<sup>f</sup></b> |                  |     |     |      |
| 32-bit floating point <sup>g</sup>                                                | 1                | 1   | 1   | 2    |
| Variant type <sup>h</sup>                                                         | 1                | 3   | 6   | 19   |

**a** Typical performance of unit with 500 MHz Pentium III processor.

**b** Measured using a VEE 5.0 program running on a 600 MHz HP Kayak, National Instruments™ GPIB card. Transferred complex S11 data, using "CALC:DATA?SDATA".

**c** Measured using a VEE 5.0 program running on a 600 MHz HP Kayak. Transferred complex S11 data, using "CALC:DATA?SDATA". Speed dependent on LAN traffic, if connected to network.

**d** Measured using a VEE 5.0 program running inside PNA Series Analyzer. Transferred complex S11 data, using "CALC:DATA?SDATA".

**e** Measured using a Visual Basic 6.0 program running inside PNA Series Analyzer. Transferred complex S11 data.

**f** Measured using a Visual Basic 6.0 program running on a 600 MHz HP Kayak. Transferred complex S11 data. Speed dependent on LAN traffic, if connected to network.

**g** Used IArray Transfer.getComplex method for 32-bit floating point.


**h** Used meas.getData method for Variant data type.

**Table 25. Recall and Sweep Speed<sup>a</sup>**


| <b>Operations</b> | <b>Number of Window(s)</b> | <b>Number of Trace(s)</b> | <b>Recall Time (ms)</b> |
|-------------------|----------------------------|---------------------------|-------------------------|
| Recall            | 1                          | 1                         | 49                      |
| Recall and Sweep  | 1                          | 1                         | 59                      |
|                   |                            |                           |                         |
| Recall            | 1                          | 2                         | 82                      |
| Recall and Sweep  | 1                          | 2                         | 96                      |
|                   |                            |                           |                         |
| Recall            | 1                          | 4                         | 159                     |
| Recall and Sweep  | 1                          | 4                         | 203                     |
|                   |                            |                           |                         |
| Recall            | 2                          | 2                         | 93                      |
| Recall and Sweep  | 2                          | 2                         | 115                     |
|                   |                            |                           |                         |
| Recall            | 3                          | 4                         | 158                     |
| Recall and Sweep  | 3                          | 4                         | 218                     |
|                   |                            |                           |                         |
| Recall            | 4                          | 4                         | 187                     |
| Recall and Sweep  | 4                          | 4                         | 247                     |
|                   |                            |                           |                         |
| Recall            | 4                          | 8                         | 340                     |
| Recall and Sweep  | 4                          | 8                         | 507                     |

aCF=177MHz, Span=200 MHz, 201 points, 35 kHz IF BW

**N3381A, N3382A, and N3383A – Simplified Test Set Block Diagram**

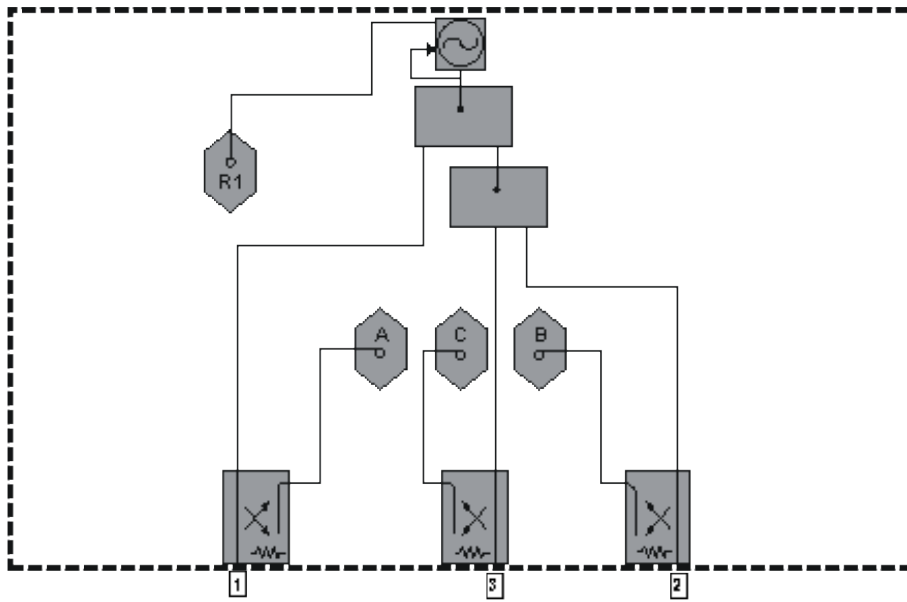

**N3381A, N3382A, and N3383A with Option 014 – Simplified Test Set Block Diagram**

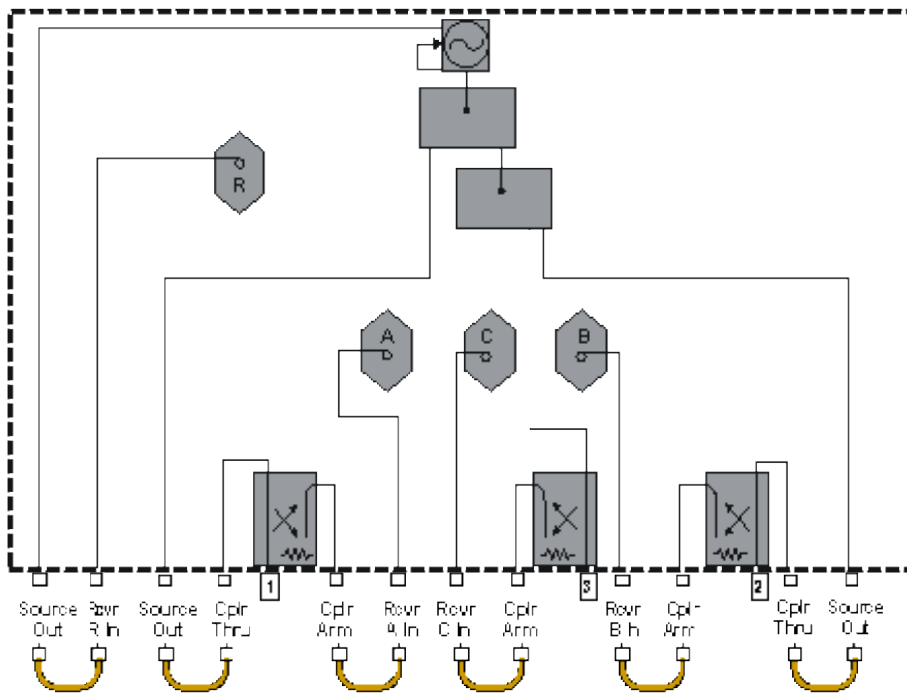

# Technical Specifications for the E8361A

(Rev. 2004-08-02)

---

This is a complete list of the E8361A network analyzer technical specifications.

- To optimize viewing of uncertainty curves, click the Maximize button.
  - To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "E8361A Specifications"
  - The uncertainty curves contained in this document apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the [equations](#) used to generate the uncertainty curves.
- 

## **Definitions**

### **Corrected System Performance**

**System Dynamic Range**

**Receiver Dynamic Range**

**185mm Connectors**

**4mm Connectors**

### **Uncorrected System Performance**

**Test Port Output**

**Test Port Input**

**Dynamic Accuracy**

**Group Delay**

 **General Information**

**Measurement Throughput Summary**

**Front-panel Jumper Specs (Option 014 only)**

**Test Set Block Diagrams**

**Test Set with Option 014 Block Diagrams**

**See Specs for other PNA models**

## **Definitions**

All specifications and characteristics apply over a 25 °C ±5 °C range (unless otherwise stated) and 90 minutes after

the instrument has been turned on.

**Specification (spec.):** Warranted performance. Specifications include guardbands to account for the expected statistical performance distribution, measurement uncertainties, and changes in performance due to environmental conditions.

**Characteristic (char.):** A performance parameter that the product is expected to meet before it leaves the factory, but that is not verified in the field and is not covered by the product warranty. A characteristic includes the same guardbands as a specification.

**Typical (typ.):** Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Nominal (nom.):** A general, descriptive term that does not imply a level of performance. It is not covered by the product warranty.

**Calibration:** The process of measuring known standards to characterize a network analyzer's systematic (repeatable) errors.

**Corrected (residual):** Indicates performance after error correction (calibration). It is determined by the quality of calibration standards and how well "known" they are, plus system repeatability, stability, and noise.

**Uncorrected (raw):** Indicates instrument performance without error correction. The uncorrected performance affects the stability of a calibration.

**Standard:** When referring to the analyzer, this includes no options unless noted otherwise.

## Corrected System Performance

The specifications in this section apply for measurements made with the E8361A analyzer with the following conditions:

- 10 Hz IF bandwidth
- No averaging applied to data

### System Dynamic Range

#### Receiver Dynamic Range

#### 185mm Connectors

#### 24mm Connectors

**Table 1.** System Dynamic Range<sup>a</sup>

| Description                                       | Specification (dB) at Test Port <sup>b</sup> | Typical (dB) at Direct Receiver Access Input <sup>c</sup> | Supplemental Information |
|---------------------------------------------------|----------------------------------------------|-----------------------------------------------------------|--------------------------|
| <b>Dynamic Range (in a 10 Hz BW)</b>              |                                              |                                                           |                          |
| <b>Standard Configuration (E8361A - Standard)</b> |                                              |                                                           |                          |
| 10 MHz to 45 MHz <sup>d</sup>                     | 61                                           | NA                                                        |                          |
| 45 MHz to 500 MHz <sup>e</sup>                    | 87                                           | NA                                                        |                          |
| 500 MHz to 750 MHz                                | 112                                          | NA                                                        |                          |

|                                                                          |     |       |                                          |
|--------------------------------------------------------------------------|-----|-------|------------------------------------------|
| 750 MHz to 2 GHz                                                         | 111 | NA    |                                          |
| 2 GHz to 10 GHz                                                          | 111 | NA    |                                          |
| 10 GHz to 24 GHz                                                         | 114 | NA    |                                          |
| 24 GHz to 30 GHz                                                         | 103 | NA    |                                          |
| 30 GHz to 40 GHz                                                         | 104 | NA    |                                          |
| 40 GHz to 45 GHz                                                         | 96  | NA    |                                          |
| 45 GHz to 50 GHz                                                         | 100 | NA    |                                          |
| 50 GHz to 60 GHz                                                         | 97  | NA    |                                          |
| 60 GHz to 67 GHz                                                         | 94  | NA    |                                          |
| 67 GHz to 70 GHz <sup>d</sup>                                            | 94  | NA    |                                          |
| <b>Configurable Test Set</b>                                             |     |       |                                          |
| <b>(E8361A - Option 014 or Option 014 and 080)</b>                       |     |       |                                          |
| 10 MHz to 45 MHz <sup>d</sup>                                            | 61  | 99    |                                          |
| 45 MHz to 500 MHz <sup>e</sup>                                           | 87  | 102   |                                          |
| 500 MHz to 750 MHz                                                       | 112 | 125.5 |                                          |
| 750 MHz to 2 GHz                                                         | 111 | 125.5 |                                          |
| 2 GHz to 10 GHz                                                          | 111 | 125   |                                          |
| 10 GHz to 24 GHz                                                         | 112 | 128   |                                          |
| 24 GHz to 30 GHz                                                         | 101 | 117.5 | Option 016 degrades performance by 2 dB. |
| 30 GHz to 40 GHz                                                         | 102 | 115   |                                          |
| 40 GHz to 45 GHz                                                         | 94  | 109   |                                          |
| 45 GHz to 50 GHz                                                         | 98  | 110.5 |                                          |
| 50 GHz to 60 GHz                                                         | 95  | 107   |                                          |
| 60 GHz to 67 GHz                                                         | 90  | 101   | Option 016 degrades performance by 3 dB. |
| 67 GHz to 70 GHz <sup>d</sup>                                            | 90  | 100   |                                          |
| <b>Configurable Test Set &amp; Extended Power Range</b>                  |     |       |                                          |
| <b>(E8361A - Option 014 &amp; UNL or Option 014 &amp; UNL &amp; 080)</b> |     |       |                                          |
| 10 MHz to 45 MHz <sup>d</sup>                                            | 61  | 99    |                                          |
| 45 MHz to 500 MHz <sup>e</sup>                                           | 87  | 102   |                                          |
| 500 MHz to 750 MHz                                                       | 112 | 125.5 |                                          |
| 750 MHz to 2 GHz                                                         | 111 | 124   |                                          |



|                               |     |       |                                          |
|-------------------------------|-----|-------|------------------------------------------|
| 2 GHz to 10 GHz               | 111 | 124   |                                          |
| 10 GHz to 24 GHz              | 112 | 125   |                                          |
| 24 GHz to 30 GHz              | 101 | 114.5 | Option 016 degrades performance by 2 dB. |
| 30 GHz to 40 GHz              | 99  | 112   |                                          |
| 40 GHz to 45 GHz              | 92  | 105   |                                          |
| 45 GHz to 50 GHz              | 94  | 106.5 |                                          |
| 50 GHz to 60 GHz              | 91  | 103   |                                          |
| 60 GHz to 67 GHz              | 84  | 95    | Option 016 degrades performance by 3 dB. |
| 67 GHz to 70 GHz <sup>d</sup> | 84  | 94    |                                          |

a The system dynamic range is calculated as the difference between the noise floor and the source maximum output power. System Dynamic Range is a specification when the source is set to Port 1, and a characteristic when the source is set to Port 2. The effective dynamic range must take measurement uncertainties and interfering signals into account as well as the insertion loss resulting from a thru cable connected between Port 1 and Port 2..

b The test port system dynamic range is calculated as the difference between the test port noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account as well as the insertion loss resulting from a thru cable connected between Port 1 and Port 2..

c The direct receiver access input system dynamic range is calculated as the difference between the receiver access input noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its damage level. When the analyzer is in segment sweep mode, the analyzer can have predefined frequency segments which will output a higher power level when the extended dynamic range is required (i.e. devices with high insertion loss), and reduced power when receiver damage may occur (i.e. devices with low insertion loss). The extended range is only available in one-path transmission measurements.

d Typical performance.

e May be limited to 100 dB at particular frequencies below 500 MHz due to spurious receiver residuals. Methods are available to regain the full dynamic range.

---

**Note:** This E8361A document does NOT provide technical specifications for Receiver Dynamic Range.

---

**Note:** This E8361A document provides technical specifications for the following calibration kits and Ecal modules only: 85056A, 85058B, N4693A, N4694A. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup.

---

**Table 10. Uncorrected System Performance<sup>a</sup>**

Specifications apply over environmental temperature of 23° ±3 °C, with < 1 °C deviation from the calibration temperature

| Description                   | Specification | Supplemental Information |
|-------------------------------|---------------|--------------------------|
| <b>Directivity</b>            |               |                          |
|                               |               | <b>typical:</b>          |
| 10 MHz to 45 MHz <sup>b</sup> | 22 dB         | 22 dB                    |
| 45 MHz to 2 GHz               | 24 dB         | 27 dB                    |
| 2 GHz to 10 GHz               | 20 dB         | 24 dB                    |
| 10 GHz to 20 GHz              | 16 dB         | 20 dB                    |
| 20 GHz to 30 GHz              | 14 dB         | 17 dB                    |

|                                  |        |                 |
|----------------------------------|--------|-----------------|
| 30 GHz to 50 GHz                 | 13 dB  | 17 dB           |
| 50 GHz to 60 GHz                 | 13 dB  | 17 dB           |
| 60 GHz to 67 GHz                 | 10 dB  | 18 dB           |
| 67 GHz to 70 GHz <sup>b</sup>    | 14 dB  | 14 dB           |
| <b>Source Match - Standard</b>   |        |                 |
|                                  |        | <b>typical:</b> |
| 10 MHz to 45 MHz <sup>b</sup>    | 7 dB   | 7 dB            |
| 45 MHz to 2 GHz                  | 18 dB  | 23 dB           |
| 2 GHz to 10 GHz                  | 14 dB  | 18 dB           |
| 10 GHz to 20 GHz                 | 12 dB  | 15 dB           |
| 20 GHz to 30 GHz                 | 8 dB   | 11.5 dB         |
| 30 GHz to 40 GHz                 | 7.5 dB | 10 dB           |
| 40 GHz to 45 GHz                 | 8 dB   | 11 dB           |
| 45 GHz to 50 GHz                 | 7 dB   | 10 dB           |
| 50 GHz to 60 GHz                 | 6 dB   | 8.5 dB          |
| 60 GHz to 67 GHz                 | 5.5 dB | 7.5 dB          |
| 67 GHz to 70 GHz <sup>b</sup>    | 7.5 dB | 7.5 dB          |
| <b>Source Match - Option 014</b> |        |                 |
|                                  |        | <b>typical:</b> |
| 10 MHz to 45 MHz <sup>b</sup>    | 7 dB   | 7 dB            |
| 45 MHz to 2 GHz                  | 17 dB  | 21 dB           |
| 2 GHz to 10 GHz                  | 12 dB  | 17 dB           |
| 10 GHz to 20 GHz                 | 11 dB  | 14 dB           |
| 20 GHz to 30 GHz                 | 10 dB  | 13 dB           |
| 30 GHz to 40 GHz                 | 8.5 dB | 11 dB           |
| 40 GHz to 45 GHz                 | 8.5 dB | 11 dB           |
| 45 GHz to 50 GHz                 | 8.5 dB | 11.5 dB         |

|                                     |        |                 |
|-------------------------------------|--------|-----------------|
| 50 GHz to 60 GHz                    | 6.5 dB | 9 dB            |
| 60 GHz to 67 GHz                    | 6 dB   | 8.5 dB          |
| 67 GHz to 70 GHz <sup>b</sup>       | 8.5 dB | 8.5 dB          |
| <b>Source Match - UNL &amp; 014</b> |        |                 |
|                                     |        | <b>typical:</b> |
| 10 MHz to 45 MHz <sup>b</sup>       | 5 dB   | 5 dB            |
| 45 MHz to 2 GHz                     | 15 dB  | 20 dB           |
| 2 GHz to 10 GHz                     | 9 dB   | 13 dB           |
| 10 GHz to 20 GHz                    | 7.5 dB | 10.5 dB         |
| 20 GHz to 30 GHz                    | 8.5 dB | 11 dB           |
| 30 GHz to 40 GHz                    | 8 dB   | 11 dB           |
| 40 GHz to 45 GHz                    | 8.5 dB | 12 dB           |
| 45 GHz to 50 GHz                    | 8 dB   | 12 dB           |
| 50 GHz to 60 GHz                    | 7 dB   | 11 dB           |
| 60 GHz to 67 GHz                    | 6 dB   | 10 dB           |
| 67 GHz to 70 GHz <sup>b</sup>       | 10 dB  | 10 dB           |
| <b>Load Match - Standard</b>        |        |                 |
|                                     |        | <b>typical:</b> |
| 10 MHz to 45 MHz <sup>b</sup>       | 5.5 dB | 5.5 dB          |
| 45 MHz to 2 GHz                     | 9 dB   | 10 dB           |
| 2 GHz to 10 GHz                     | 9 dB   | 11 dB           |
| 10 GHz to 20 GHz                    | 8.5 dB | 10 dB           |
| 20 GHz to 30 GHz                    | 7 dB   | 9 dB            |
| 30 GHz to 40 GHz                    | 6 dB   | 8 dB            |
| 40 GHz to 45 GHz                    | 6.5 dB | 9 dB            |
| 45 GHz to 50 GHz                    | 6.5 dB | 8.5 dB          |
| 50 GHz to 60 GHz                    | 5.5 dB | 7.5 dB          |

|                                          |        |                 |
|------------------------------------------|--------|-----------------|
| 60 GHz to 67 GHz                         | 5.5 dB | 7.5 dB          |
| 67 GHz to 70 GHz <sup>b</sup>            | 5 dB   | 5 dB            |
| <b>Load Match - Option 014</b>           |        |                 |
|                                          |        | <b>typical:</b> |
| 10 MHz to 45 MHz <sup>b</sup>            | 5.5 dB | 5.5 dB          |
| 45 MHz to 2 GHz                          | 8.5 dB | 10 dB           |
| 2 GHz to 10 GHz                          | 8 dB   | 10 dB           |
| 10 GHz to 20 GHz                         | 8 dB   | 10 dB           |
| 20 GHz to 30 GHz                         | 7.5 dB | 10 dB           |
| 30 GHz to 40 GHz                         | 7 dB   | 9.5 dB          |
| 40 GHz to 45 GHz                         | 7.5 dB | 9.5 dB          |
| 45 GHz to 50 GHz                         | 7.5 dB | 10 dB           |
| 50 GHz to 60 GHz                         | 6 dB   | 8.5 dB          |
| 60 GHz to 67 GHz                         | 6 dB   | 8.5 dB          |
| 67 GHz to 70 GHz <sup>b</sup>            | 5 dB   | 5 dB            |
| <b>Load Match - Option UNL &amp; 014</b> |        |                 |
|                                          |        | <b>typical:</b> |
| 10 MHz to 45 MHz <sup>b</sup>            | 6 dB   | 6 dB            |
| 45 MHz to 2 GHz                          | 8.5 dB | 10 dB           |
| 2 GHz to 10 GHz                          | 7 dB   | 9 dB            |
| 10 GHz to 20 GHz                         | 6 dB   | 9 dB            |
| 20 GHz to 30 GHz                         | 7.5 dB | 11 dB           |
| 30 GHz to 40 GHz                         | 8 dB   | 11.5 dB         |
| 40 GHz to 45 GHz                         | 8 dB   | 12 dB           |
| 45 GHz to 50 GHz                         | 8 dB   | 12 dB           |
| 50 GHz to 60 GHz                         | 7.5 dB | 11.5 dB         |
| 60 GHz to 67 GHz                         | 6 dB   | 10 dB           |

|                                          |         |                 |
|------------------------------------------|---------|-----------------|
| 67 GHz to 70 GHz <sup>b</sup>            | 13 dB   | 13 dB           |
| <b>Reflection Tracking</b>               |         |                 |
|                                          |         | <b>typical:</b> |
| 10 MHz to 45 MHz                         |         | ±1.5 dB         |
| 45 MHz to 20 GHz                         |         | ±1.5 dB         |
| 20 GHz to 40 GHz                         |         | ±2.0 dB         |
| 40 GHz to 50 GHz                         |         | ±2.0 dB         |
| 50 GHz to 67 GHz                         |         | ±3.0 dB         |
| 67 GHz to 70 GHz                         |         | ±4.5 dB         |
| <b>Transmission Tracking<sup>c</sup></b> |         |                 |
|                                          |         | <b>typical:</b> |
| 10 MHz to 45 MHz                         |         | ±1.5 dB         |
| 45 MHz to 20 GHz                         |         | ±1.5 dB         |
| 20 GHz to 40 GHz                         |         | ±2.0 dB         |
| 40 GHz to 50 GHz                         |         | ±2.0 dB         |
| 50 GHz to 67 GHz                         |         | ±3.0 dB         |
| 67 GHz to 70 GHz                         |         | ±4.5 dB         |
| <b>Crosstalk<sup>d</sup> - Standard</b>  |         |                 |
| 10 MHz to 45 MHz <sup>b</sup>            | -63 dB  |                 |
| 45 MHz to 500 MHz                        | -87 dB  |                 |
| 500 MHz to 2 GHz                         | -110 dB |                 |
| 2 GHz to 10 GHz                          | -105 dB |                 |
| 10 GHz to 24 GHz                         | -111 dB |                 |
| 24 GHz to 30 GHz                         | -106 dB |                 |
| 30 GHz to 40 GHz                         | -104 dB |                 |
| 40 GHz to 45 GHz                         | -98 dB  |                 |
| 45 GHz to 50 GHz                         | -100 dB |                 |

|                                                     |         |                                                       |
|-----------------------------------------------------|---------|-------------------------------------------------------|
| 50 GHz to 60 GHz                                    | -97 dB  |                                                       |
| 60 GHz to 67 GHz                                    | -94 dB  |                                                       |
| 67 GHz to 70 GHz <sup>b</sup>                       | -94 dB  |                                                       |
| <b>Crosstalk<sup>d</sup> - Option 014</b>           |         |                                                       |
|                                                     |         | <b>typical</b> (for Option 080 enabled <sup>e</sup> ) |
| 10 MHz to 45 MHz <sup>b</sup>                       | -63 dB  | -63 dB                                                |
| 45 MHz to 500 MHz                                   | -87 dB  | -87 dB                                                |
| 500 MHz to 2 GHz                                    | -110 dB | -110 dB                                               |
| 2 GHz to 10 GHz                                     | -105 dB | -105 dB                                               |
| 10 GHz to 24 GHz                                    | -111 dB | -111 dB                                               |
| 24 GHz to 30 GHz                                    | -104 dB | -104 dB                                               |
| 30 GHz to 40 GHz                                    | -102 dB | -102 dB                                               |
| 40 GHz to 45 GHz                                    | -96 dB  | -96 dB                                                |
| 45 GHz to 50 GHz                                    | -98 dB  | -98 dB                                                |
| 50 GHz to 60 GHz                                    | -95 dB  | -95 dB                                                |
| 60 GHz to 67 GHz                                    | -90 dB  | -90 dB                                                |
| 67 GHz to 70 GHz <sup>b</sup>                       | -90 dB  | -90 dB                                                |
| <b>Crosstalk<sup>d</sup> - Option 014 &amp; UNL</b> |         |                                                       |
|                                                     |         | <b>typical</b> (for Option 080 enabled <sup>e</sup> ) |
| 10 MHz to 45 MHz <sup>b</sup>                       | -63 dB  | -63 dB                                                |
| 45 MHz to 500 MHz                                   | -87 dB  | -87 dB                                                |
| 500 MHz to 2 GHz                                    | -110 dB | -110 dB                                               |
| 2 GHz to 10 GHz                                     | -104 dB | -104 dB                                               |
| 10 GHz to 24 GHz                                    | -108 dB | -108 dB                                               |
| 24 GHz to 30 GHz                                    | -101 dB | -101 dB                                               |
| 30 GHz to 40 GHz                                    | -99 dB  | -99 dB                                                |
| 40 GHz to 45 GHz                                    | -92 dB  | -92 dB                                                |

|                               |        |        |
|-------------------------------|--------|--------|
| 45 GHz to 50 GHz              | -94 dB | -94 dB |
| 50 GHz to 60 GHz              | -91 dB | -91 dB |
| 60 GHz to 67 GHz              | -84 dB | -84 dB |
| 67 GHz to 70 GHz <sup>b</sup> | -84 dB | -84 dB |

a Specifications apply over environment temperature of 23°C +/- 3°C, with less than 1°C deviation from the calibration temperature.

b Typical performance.

c Transmission tracking performance noted here is normalized to the insertion loss characteristics of the cable used so that the indicated performance is independent of the cable used.

d Measurement conditions: normalized to a thru, measured with two shorts, 10 Hz IF bandwidth, averaging factor of 16, alternate mode, source power set to the lesser of the maximum power out or the maximum receiver power.

e 0 Hz offset.

**Table 11. Test Port Output**

| Description                             | Specification                                   |                         | Supplemental                                                        |
|-----------------------------------------|-------------------------------------------------|-------------------------|---------------------------------------------------------------------|
| <b>Frequency Range</b>                  |                                                 |                         |                                                                     |
|                                         | <b>Standard</b>                                 | <b>Options</b>          |                                                                     |
| E8361A                                  | 45 MHz to 67 GHz<br>(Operates 10 MHz to 70 GHz) |                         |                                                                     |
| <b>Nominal Power<sup>c</sup></b>        |                                                 |                         |                                                                     |
|                                         | <b>Std and Options without UNL</b>              | <b>Options with UNL</b> |                                                                     |
| E8361A                                  | -15 dBm                                         | -17 dBm                 |                                                                     |
| <b>Frequency Resolution</b>             |                                                 |                         |                                                                     |
|                                         | 1 Hz                                            |                         |                                                                     |
| <b>CW Accuracy</b>                      |                                                 |                         |                                                                     |
|                                         | +/-1 ppm                                        |                         |                                                                     |
| <b>Frequency Stability</b>              |                                                 |                         |                                                                     |
|                                         |                                                 |                         | +/-0.05 ppm. -10° to 70° C, typical; +/-0.1 ppm/yr maximum, typical |
| <b>Power Level Accuracy<sup>a</sup></b> |                                                 |                         |                                                                     |
|                                         | <b>Standard</b>                                 | <b>Opt 014</b>          | <b>Opt 014 &amp; UNL</b>                                            |

|                                                                                                                                                                |                                          |                |                          |                                                                   |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------|----------------|--------------------------|-------------------------------------------------------------------|
| 10 MHz to 45 MHz <sup>b</sup>                                                                                                                                  | +/-1.5 dB                                | +/-1.5 dB      | +/-1.5 dB                | Variation from nominal power in range 0 (step attenuator at 0 dB) |
| 45 MHz to 10 GHz                                                                                                                                               | +/-1.5 dB                                | +/-1.5 dB      | +/-1.5 dB                |                                                                   |
| 10 GHz to 20 GHz                                                                                                                                               | +/-1.5 dB                                | +/-1.5 dB      | +/-2.0 dB                |                                                                   |
| 20 GHz to 30 GHz                                                                                                                                               | +/-2.0 dB                                | +/-2.0 dB      | +/-2.5 dB                |                                                                   |
| 30 GHz to 40 GHz                                                                                                                                               | +/-3.0 dB                                | +/-3.0 dB      | +/-3 dB                  |                                                                   |
| 40 GHz to 45 GHz                                                                                                                                               | +/-3.0 dB                                | +/-3.0 dB      | +/-3 dB                  |                                                                   |
| 45 GHz to 50 GHz                                                                                                                                               | +/-3.5 dB                                | +/-3.5 dB      | +/-3.5 dB                |                                                                   |
| 50 GHz to 60 GHz                                                                                                                                               | +/-4.0 dB                                | +/-4.0 dB      | +/-4.0 dB                |                                                                   |
| 60 GHz to 67 GHz                                                                                                                                               | +/-4.0 dB                                | +/-4.0 dB      | +/-4.5 dB                |                                                                   |
| 67 GHz to 70 GHz <sup>b</sup>                                                                                                                                  | +/-4.0 dB                                | +/-4.0 dB      | +/-4.5 dB                |                                                                   |
| <b>Power Level Linearity<sup>d</sup></b>                                                                                                                       |                                          |                |                          |                                                                   |
|                                                                                                                                                                |                                          |                |                          | <b>Any Option</b>                                                 |
| Test reference is at the nominal power level (step attenuator at 0 dB)                                                                                         |                                          |                |                          |                                                                   |
| 10 MHz to 45 MHz <sup>b</sup>                                                                                                                                  | +/-1.0 dB for power<=-5 dBm <sup>g</sup> |                |                          |                                                                   |
| 45 MHz to 67 GHz                                                                                                                                               | +/-1.0 dB for power<=-5 dBm <sup>g</sup> |                |                          |                                                                   |
| 67 GHz to 70 GHz <sup>b</sup>                                                                                                                                  | +/-1.0 dB for power<=-5 dBm <sup>g</sup> |                |                          |                                                                   |
| <b>Power Range<sup>a,e,f</sup></b>                                                                                                                             |                                          |                |                          |                                                                   |
| <b>Note: If power is set above the maximum specified leveled power, the test port output signal may show non-linear effects that are dependent on the DUT.</b> |                                          |                |                          |                                                                   |
|                                                                                                                                                                | <b>Standard</b>                          | <b>Opt 014</b> | <b>Opt 014 &amp; UNL</b> |                                                                   |
| 10 MHz to 45 MHz <sup>b</sup>                                                                                                                                  | -25 to -9 dBm                            | -25 to -9 dBm  | -75 to -9 dBm            |                                                                   |



|                                |                 |                |                          |                                                                                                       |
|--------------------------------|-----------------|----------------|--------------------------|-------------------------------------------------------------------------------------------------------|
| 45 MHz to 500 MHz              | -25 to -3 dBm   | -25 to -3 dBm  | -75 to -3 dBm            |                                                                                                       |
| 500 MHz to 750 MHz             | -25 to 0 dBm    | -25 to 0 dBm   | -75 to 0 dBm             |                                                                                                       |
| 750 MHz to 10 GHz              | -27 to -1 dBm   | -27 to -1 dBm  | -77 to -1 dBm            |                                                                                                       |
| 10 GHz to 30 GHz               | -27 to -2 dBm   | -27 to -3 dBm  | -77 to -3 dBm            |                                                                                                       |
| 30 GHz to 40 GHz               | -27 to -1 dBm   | -27 to -2 dBm  | -77 to -5 dBm            |                                                                                                       |
| 40 GHz to 45 GHz               | -27 to -7 dBm   | -27 to -8 dBm  | -77 to -10 dBm           |                                                                                                       |
| 45 GHz to 50 GHz               | -27 to -1 dBm   | -27 to -2 dBm  | -77 to -6 dBm            |                                                                                                       |
| 50 GHz to 60 GHz               | -27 to -3 dBm   | -27 to -4 dBm  | -77 to -8 dBm            |                                                                                                       |
| 60 GHz to 67 GHz               | -27 to -5 dBm   | -27 to -7 dBm  | -77 to -13 dBm           |                                                                                                       |
| 67 GHz to 70 GHz <sup>b</sup>  | -27 to -5 dBm   | -27 to -7 dBm  | -77 to -13 dBm           |                                                                                                       |
| <b>Power Sweep Range (ALC)</b> |                 |                |                          |                                                                                                       |
|                                | <b>Standard</b> | <b>Opt 014</b> | <b>Opt 014 &amp; UNL</b> | ALC range starts at maximum leveled output power and decreases by power level indicated in the table. |
| 10 MHz to 45 MHz <sup>b</sup>  | 16 dB           | 16 dB          | 16 dB                    |                                                                                                       |
| 45 MHz to 500 MHz              | 22 dB           | 22 dB          | 22 dB                    |                                                                                                       |
| 500 MHz to 750 MHz             | 25 dB           | 25 dB          | 25 dB                    |                                                                                                       |
| 750 GHz to 10 GHz              | 26 dB           | 26 dB          | 26 dB                    |                                                                                                       |
| 10 GHz to 30 GHz               | 25 dB           | 24 dB          | 24 dB                    |                                                                                                       |

|                                                                                             |         |       |       |                   |
|---------------------------------------------------------------------------------------------|---------|-------|-------|-------------------|
| 30 GHz to 40 GHz                                                                            | 26 dB   | 25 dB | 22 dB |                   |
| 40 GHz to 45 GHz                                                                            | 20 dB   | 19 dB | 17 dB |                   |
| 45 GHz to 50 GHz                                                                            | 26 dB   | 25 dB | 21 dB |                   |
| 50 GHz to 60 GHz                                                                            | 24 dB   | 23 dB | 19 dB |                   |
| 60 GHz to 67 GHz                                                                            | 22 dB   | 20 dB | 14 dB |                   |
| 67 GHz to 70 GHz <sup>b</sup>                                                               | 22 dB   | 20 dB | 14 dB |                   |
| <b>Power Resolution</b>                                                                     |         |       |       |                   |
|                                                                                             | 0.01 dB |       |       |                   |
| <b>Phase Noise</b>                                                                          |         |       |       |                   |
|                                                                                             |         |       |       | <b>Any Option</b> |
| <b>10 kHz offset from center frequency, nominal power at test port</b>                      |         |       |       |                   |
|                                                                                             |         |       |       | <b>typical:</b>   |
| 10 MHz to 45 MHz                                                                            |         |       |       | -80 dBc           |
| 45 MHz to 10 GHz                                                                            |         |       |       | -70 dBc           |
| 10 GHz to 24 GHz                                                                            |         |       |       | -60 dBc           |
| 24 GHz to 70 GHz                                                                            |         |       |       | -55 dBc           |
| <b>10 kHz offset from center frequency, nominal power at test port - Option 080 enabled</b> |         |       |       |                   |
|                                                                                             |         |       |       | <b>typical:</b>   |
| 10 MHz to 45 MHz                                                                            |         |       |       | -80 dBc           |
| 45 MHz to 10 GHz                                                                            |         |       |       | -70 dBc           |
| 10 GHz to 24 GHz                                                                            |         |       |       | -60 dBc           |

|                                                                                              |  |  |  |                 |
|----------------------------------------------------------------------------------------------|--|--|--|-----------------|
| 24 GHz to<br>70 GHz                                                                          |  |  |  | -55 dBc         |
| <b>100 kHz offset from center frequency, nominal power at test port</b>                      |  |  |  |                 |
|                                                                                              |  |  |  | <b>typical:</b> |
| 10 MHz to<br>45 MHz                                                                          |  |  |  | -90 dBc         |
| 45 MHz to<br>10 GHz                                                                          |  |  |  | -90 dBc         |
| 10 GHz to<br>24 GHz                                                                          |  |  |  | -85 dBc         |
| 24 GHz to<br>70 GHz                                                                          |  |  |  | -75 dBc         |
| <b>100 kHz offset from center frequency, nominal power at test port - Option 080 enabled</b> |  |  |  |                 |
|                                                                                              |  |  |  | <b>typical:</b> |
| 10 MHz to<br>45 MHz                                                                          |  |  |  | -85 dBc         |
| 45 MHz to<br>10 GHz                                                                          |  |  |  | -80 dBc         |
| 10 GHz to<br>24 GHz                                                                          |  |  |  | -70 dBc         |
| 24 GHz to<br>70 GHz                                                                          |  |  |  | -60 dBc         |
| <b>1 MHz offset from center frequency, nominal power at test port</b>                        |  |  |  |                 |
|                                                                                              |  |  |  | <b>typical:</b> |
| 10 MHz to<br>45 MHz                                                                          |  |  |  | -115 dBc        |
| 45 MHz to<br>10 GHz                                                                          |  |  |  | -110 dBc        |
| 10 GHz to<br>24 GHz                                                                          |  |  |  | -105 dBc        |
| 24 GHz to<br>70 GHz                                                                          |  |  |  | -95 dBc         |
| <b>1 MHz offset from center frequency, nominal power at test port - Option 080 enabled</b>   |  |  |  |                 |
|                                                                                              |  |  |  | <b>typical:</b> |

|                                                        |  |  |  |                                               |
|--------------------------------------------------------|--|--|--|-----------------------------------------------|
| 10 MHz to 45 MHz                                       |  |  |  | -110 dBc                                      |
| 45 MHz to 10 GHz                                       |  |  |  | -105 dBc                                      |
| 10 GHz to 24 GHz                                       |  |  |  | -95 dBc                                       |
| 24 GHz to 70 GHz                                       |  |  |  | -85 dBc                                       |
| <b>Harmonics (2nd or 3rd)</b>                          |  |  |  |                                               |
|                                                        |  |  |  | <b>Any Option</b>                             |
|                                                        |  |  |  | <b>typical:</b>                               |
| 10 MHz to 500 MHz                                      |  |  |  | -10 dBc                                       |
| 500 MHz to 10 GHz                                      |  |  |  | -15 dBc                                       |
| 10 GHz to 24 GHz                                       |  |  |  | -23 dBc                                       |
| 24 GHz to 50 GHz                                       |  |  |  | -16 dBc                                       |
| 50 GHz to 60 GHz                                       |  |  |  | -13 dBc                                       |
| 60 GHz to 70 GHz                                       |  |  |  | -19 dBc                                       |
| <b>Non-Harmonic Spurious (at Nominal Output Power)</b> |  |  |  |                                               |
| 10 MHz to 20 GHz                                       |  |  |  | -50 dBc typical, for offset frequency > 1 kHz |
| 20 GHz to 70 GHz                                       |  |  |  | -30 dBc typical, for offset frequency > 1 kHz |

a Test port output is a specification when the source is set to Port 1, and a characteristic when the source is set to Port 2.

b Typical performance.

c Preset power.

d Power Level Linearity is a specification when the source is set to Port 1, and a typical when the source is set to Port 2.

e Test port power is specified into nominal 50 ohms.

f Power to which the source can be set and phase lock is assured.

g +/-1.6 dB for power > -5 dBm.

**Table 12: Test Port Input**

| Description                              | Specification   |                      | Supplemental                                    |
|------------------------------------------|-----------------|----------------------|-------------------------------------------------|
|                                          | Standard or UNL | Opt 014 or 014 & UNL |                                                 |
| <b>Test Port Noise Floor<sup>1</sup></b> |                 |                      |                                                 |
| <b>10 Hz IF Bandwidth</b>                |                 |                      |                                                 |
| 10 MHz to 45 MHz <sup>2</sup>            | <-70 dBm        | <-70 dBm             |                                                 |
| 45 MHz to 500 MHz <sup>3, 4</sup>        | <-90 dBm        | <-90 dBm             |                                                 |
| 500 MHz to 2 GHz                         | <-112 dBm       | <-112 dBm            |                                                 |
| 2 GHz to 10 GHz                          | <-112 dBm       | <-112 dBm            |                                                 |
| 10 GHz to 24 GHz                         | <-116 dBm       | <-115 dBm            |                                                 |
| 24 GHz to 30 GHz                         | <-105 dBm       | <-104 dBm            | <u>Option 016</u> degrades performance by 2 dB. |
| 30 GHz to 40 GHz                         | <-105 dBm       | <-104 dBm            |                                                 |
| 40 GHz to 45 GHz                         | <-103 dBm       | <-102 dBm            |                                                 |
| 45 GHz to 50 GHz                         | <-101 dBm       | <-100 dBm            |                                                 |
| 50 GHz to 60 GHz                         | <-100 dBm       | <-99 dBm             |                                                 |
| 60 GHz to 67 GHz                         | <-99 dBm        | <-97 dBm             | <u>Option 016</u> degrades performance by 3 dB. |
| 67 GHz to 70 GHz <sup>2</sup>            | <-99 dBm        | <-97 dBm             |                                                 |
| <b>1 KHz IF Bandwidth</b>                |                 |                      |                                                 |
| 10 MHz to 45 MHz <sup>2</sup>            | <-50 dBm        | <-50 dBm             |                                                 |
| 45 MHz to 500 MHz <sup>3, 4</sup>        | <-70 dBm        | <-70 dBm             |                                                 |
| 500 MHz to 2 GHz                         | <-92 dBm        | <-92 dBm             |                                                 |
| 2 GHz to 10 GHz                          | <-92 dBm        | <-92 dBm             |                                                 |
| 10 GHz to 24 GHz                         | <-96 dBm        | <-95 dBm             |                                                 |

|                                                                         |          |                                                 |                                                 |
|-------------------------------------------------------------------------|----------|-------------------------------------------------|-------------------------------------------------|
| 24 GHz to 30 GHz                                                        | <-85 dBm | <-84 dBm                                        | <u>Option 016</u> degrades performance by 2 dB. |
| 30 GHz to 40 GHz                                                        | <-85 dBm | <-84 dBm                                        |                                                 |
| 40 GHz to 45 GHz                                                        | <-83 dBm | <-82 dBm                                        |                                                 |
| 45 GHz to 50 GHz                                                        | <-81 dBm | <-80 dBm                                        |                                                 |
| 50 GHz to 60 GHz                                                        | <-80 dBm | <-79 dBm                                        |                                                 |
| 60 GHz to 67 GHz                                                        | <-79 dBm | <-77 dBm                                        | <u>Option 016</u> degrades performance by 3 dB. |
| 67 GHz to 70 GHz <sup>2</sup>                                           | <-79 dBm | <-77 dBm                                        |                                                 |
| <b>Test Port Noise Floor<sup>1</sup> Option 080 enabled<sup>5</sup></b> |          |                                                 |                                                 |
|                                                                         |          |                                                 | <b>Option 014 or 014 &amp; UNL (typical)</b>    |
| <b>10 Hz IF Bandwidth</b>                                               |          |                                                 |                                                 |
| 10 MHz to 45 MHz                                                        |          |                                                 | <-70 dBm                                        |
| 45 MHz to 500 MHz <sup>3, 4</sup>                                       |          |                                                 | <-90 dBm                                        |
| 500 MHz to 2 GHz                                                        |          |                                                 | <-112 dBm                                       |
| 2 GHz to 10 GHz                                                         |          |                                                 | <-112 dBm                                       |
| 10 GHz to 24 GHz                                                        |          |                                                 | <-115 dBm                                       |
| 24 GHz to 30 GHz                                                        |          | <u>Option 016</u> degrades performance by 2 dB. | <-104 dBm                                       |
| 30 GHz to 40 GHz                                                        |          |                                                 | <-104 dBm                                       |
| 40 GHz to 45 GHz                                                        |          |                                                 | <-102 dBm                                       |
| 45 GHz to 50 GHz                                                        |          |                                                 | <-100 dBm                                       |
| 50 GHz to 60 GHz                                                        |          |                                                 | <-99 dBm                                        |
| 60 GHz to 67 GHz                                                        |          | <u>Option 016</u> degrades performance by 3 dB. | <-97 dBm                                        |
| 67 GHz to 70 GHz                                                        |          |                                                 | <-97 dBm                                        |
| <b>1 KHz IF Bandwidth</b>                                               |          |                                                 |                                                 |
|                                                                         |          |                                                 | <b>typical:</b>                                 |
| 10 MHz to 45 MHz                                                        |          |                                                 | <-50 dBm                                        |
| 45 MHz to 500 MHz <sup>3, 4</sup>                                       |          |                                                 | <-70 dBm                                        |

|                                                             |                 |                                          |                                              |
|-------------------------------------------------------------|-----------------|------------------------------------------|----------------------------------------------|
| 500 MHz to 2 GHz                                            |                 |                                          | <-92 dBm                                     |
| 2 GHz to 10 GHz                                             |                 |                                          | <-92 dBm                                     |
| 10 GHz to 24 GHz                                            |                 |                                          | <-95 dBm                                     |
| 24 GHz to 30 GHz                                            |                 | Option 016 degrades performance by 2 dB. | <-84 dBm                                     |
| 30 GHz to 40 GHz                                            |                 |                                          | <-84 dBm                                     |
| 40 GHz to 45 GHz                                            |                 |                                          | <-82 dBm                                     |
| 45 GHz to 50 GHz                                            |                 |                                          | <-80 dBm                                     |
| 50 GHz to 60 GHz                                            |                 |                                          | <-79 dBm                                     |
| 60 GHz to 67 GHz                                            |                 | Option 016 degrades performance by 3 dB. | <-77 dBm                                     |
| 67 GHz to 70 GHz                                            |                 |                                          | <-77 dBm                                     |
| <b>Direct Receiver Access Input Noise Floor<sup>1</sup></b> |                 |                                          |                                              |
|                                                             | <b>Standard</b> |                                          | <b>Option 014 or 014 &amp; UNL (typical)</b> |
| <b>10 Hz IF Bandwidth</b>                                   |                 |                                          |                                              |
| 10 MHz to 45 MHz <sup>2</sup>                               |                 |                                          | <-106 dBm                                    |
| 45 MHz to 500 MHz <sup>3, 4</sup>                           |                 |                                          | <-105 dBm                                    |
| 500 MHz to 2 GHz                                            |                 |                                          | <-125.5 dBm                                  |
| 2 GHz to 10 GHz                                             |                 |                                          | <-125 dBm                                    |
| 10 GHz to 24 GHz                                            |                 |                                          | <-128 dBm                                    |
| 24 GHz to 30 GHz                                            |                 | Option 016 degrades performance by 2 dB. | <-117.5 dBm                                  |
| 30 GHz to 40 GHz                                            |                 |                                          | <-117 dBm                                    |
| 40 GHz to 45 GHz                                            |                 |                                          | <-115 dBm                                    |
| 45 GHz to 50 GHz                                            |                 |                                          | <-112.5 dBm                                  |
| 50 GHz to 60 GHz                                            |                 |                                          | <-111 dBm                                    |
| 60 GHz to 67 GHz                                            |                 | Option 016 degrades performance by 3 dB  | <-108 dBm                                    |
| 67 GHz to 70 GHz <sup>2</sup>                               |                 |                                          | <-107 dBm                                    |
| <b>1 KHz IF Bandwidth</b>                                   |                 |                                          |                                              |

|                                                                                              |                 |                                                 |                   |
|----------------------------------------------------------------------------------------------|-----------------|-------------------------------------------------|-------------------|
| 10 MHz to 45 MHz <sup>2</sup>                                                                |                 |                                                 | <-86 dBm          |
| 45 MHz to 500 MHz <sup>3, 4</sup>                                                            |                 |                                                 | <-85 dBm          |
| 500 MHz to 2 GHz                                                                             |                 |                                                 | <-105.5 dBm       |
| 2 GHz to 10 GHz                                                                              |                 |                                                 | <-105 dBm         |
| 10 GHz to 24 GHz                                                                             |                 |                                                 | <-108 dBm         |
| 24 GHz to 30 GHz                                                                             |                 | <u>Option 016</u> degrades performance by 2 dB. | <-97.5 dBm        |
| 30 GHz to 40 GHz                                                                             |                 |                                                 | <-97 dBm          |
| 40 GHz to 45 GHz                                                                             |                 |                                                 | <-95 dBm          |
| 45 GHz to 50 GHz                                                                             |                 |                                                 | <-92.5 dBm        |
| 50 GHz to 60 GHz                                                                             |                 |                                                 | <-91 dBm          |
| 60 GHz to 67 GHz                                                                             |                 | <u>Option 016</u> degrades performance by 3 dB. | <-88 dBm          |
| 67 GHz to 70 GHz <sup>2</sup>                                                                |                 |                                                 | <-87 dBm          |
| <b>Direct Receiver Access Input Noise Floor<sup>1</sup> - Option 080 enabled<sup>5</sup></b> |                 |                                                 |                   |
|                                                                                              | <b>Standard</b> |                                                 | <b>Option 014</b> |
| <b>10 Hz IF Bandwidth</b>                                                                    |                 |                                                 |                   |
|                                                                                              |                 |                                                 | <b>typical:</b>   |
| 10 MHz to 45 MHz <sup>2</sup>                                                                |                 |                                                 | <-106 dBm         |
| 45 MHz to 500 MHz <sup>3, 4</sup>                                                            |                 |                                                 | <-105 dBm         |
| 500 MHz to 2 GHz                                                                             |                 |                                                 | <-125.5 dBm       |
| 2 GHz to 10 GHz                                                                              |                 |                                                 | <-125 dBm         |
| 10 GHz to 24 GHz                                                                             |                 |                                                 | <-128 dBm         |
| 24 GHz to 30 GHz                                                                             |                 | <u>Option 016</u> degrades performance by 2 dB. | <-117.5 dBm       |
| 30 GHz to 40 GHz                                                                             |                 |                                                 | <-117 dBm         |
| 40 GHz to 45 GHz                                                                             |                 |                                                 | <-115 dBm         |
| 45 GHz to 50 GHz                                                                             |                 |                                                 | <-112.5 dBm       |
| 50 GHz to 60 GHz                                                                             |                 |                                                 | <-111 dBm         |



|                                   |  |                                          |                 |
|-----------------------------------|--|------------------------------------------|-----------------|
| 60 GHz to 67 GHz                  |  | Option 016 degrades performance by 3 dB. | <-108 dBm       |
| 67 GHz to 70 GHz <sup>2</sup>     |  |                                          | <-107 dBm       |
| <b>1 KHz IF Bandwidth</b>         |  |                                          |                 |
|                                   |  |                                          | <b>typical:</b> |
| 10 MHz to 45 MHz <sup>2</sup>     |  |                                          | <-86 dBm        |
| 45 MHz to 500 MHz <sup>3, 4</sup> |  |                                          | <-85 dBm        |
| 500 MHz to 2 GHz                  |  |                                          | <-105.5 dBm     |
| 2 GHz to 10 GHz                   |  |                                          | <-105 dBm       |
| 10 GHz to 24 GHz                  |  |                                          | <-108 dBm       |
| 24 GHz to 30 GHz                  |  | Option 016 degrades performance by 2 dB. | <-97.5 dBm      |
| 30 GHz to 40 GHz                  |  |                                          | <-97 dBm        |
| 40 GHz to 45 GHz                  |  |                                          | <-95 dBm        |
| 45 GHz to 50 GHz                  |  |                                          | <-92.5 dBm      |
| 50 GHz to 60 GHz                  |  |                                          | <-91 dBm        |
| 60 GHz to 67 GHz                  |  | Option 016 degrades performance by 3 dB. | <-88 dBm        |
| 67 GHz to 70 GHz <sup>2</sup>     |  |                                          | <-87 dBm        |

**Receiver Compression Level (measured at test ports)**

|                                   | Specifications                                          |                                                         |                                                      | Supplemental Information                                |
|-----------------------------------|---------------------------------------------------------|---------------------------------------------------------|------------------------------------------------------|---------------------------------------------------------|
|                                   | Standard                                                | Option 014                                              | 014 & UNL                                            | Typical                                                 |
| 10 MHz to 45 MHz <sup>2, 6</sup>  | negligible                                              |                                                         |                                                      |                                                         |
| 45 MHz to 500 MHz <sup>6, 7</sup> | <0.1 dB at -9.5 dBm <sup>8</sup> and <0.25 dB at -3 dBm | <0.1 dB at -4.0 dBm <sup>8</sup> and <0.25 dB at +3 dBm |                                                      | <0.1 dB at +0.5 dBm <sup>8</sup> and <0.25 dB at +8 dBm |
| 500 MHz to 5 GHz                  | <0.1 dB at -8 dBm <sup>8</sup> and <0.25 dB at -1 dBm   | <0.1 dB at -8 dBm <sup>8</sup> and <0.25 dB at -1 dBm   | <0.1 dB at -7 dBm <sup>8</sup> and <0.25 dB at 0 dBm | <0.1 dB at -4.0 dBm <sup>8</sup> and <0.25 dB at +3 dBm |

|                               |                                                          |                                                         |                                                         |                                                                         |
|-------------------------------|----------------------------------------------------------|---------------------------------------------------------|---------------------------------------------------------|-------------------------------------------------------------------------|
| 5 GHz to 30 GHz               | <0.1 dB at -8.5 dBm <sup>8</sup> and <0.25 dB at -2 dBm  | <0.1 dB at -9 dBm <sup>8</sup> and <0.25 dB at -2 dBm   | <0.1 dB at -6 dBm <sup>8</sup> and <0.25 dB at +1 dBm   | <0.1 dB at -1.0 dBm <sup>8</sup> and <0.25 dB at +6 dBm                 |
| 30 GHz to 67 GHz              | <0.1 dB at -10.5 dBm <sup>8</sup> and <0.15 dB at -7 dBm | <0.1 dB at -6.0 dBm <sup>8</sup> and <0.15 dB at -4 dBm | <0.1 dB at -9.5 dBm <sup>8</sup> and <0.15 dB at -6 dBm | <0.1 dB at -2.0 dBm <sup>8, 9</sup> and <0.15 dB at +2 dBm <sup>9</sup> |
| 67 GHz to 70 GHz <sup>2</sup> | NA                                                       |                                                         |                                                         |                                                                         |

### System Compression Level

|  | Standard                     | Option 014 or 014 & UNL |                                            |
|--|------------------------------|-------------------------|--------------------------------------------|
|  | maximum leveled output power |                         | See <a href="#">dynamic accuracy table</a> |

### Third Order Intercept<sup>10</sup> - Tone spacing from 100 kHz - 5 MHz

|                   |  |  | Any Option |
|-------------------|--|--|------------|
|                   |  |  | typical    |
| 10 MHz to 500 MHz |  |  | +30 dBm    |
| 500 MHz to 24 GHz |  |  | +24 dBm    |
| 24 GHz to 40 GHz  |  |  | +23 dBm    |
| 40 to 50 GHz      |  |  | +24 dBm    |
| 50 to 67 GHz      |  |  | +26 dBm    |

### Third Order Intercept<sup>10</sup> - Tone spacing from 5 MHz - 20 MHz

|                   |  |  | Any Option |
|-------------------|--|--|------------|
|                   |  |  | typical    |
| 10 MHz to 500 MHz |  |  | NA         |
| 500 MHz to 24 GHz |  |  | +20 dBm    |
| 24 GHz to 40 GHz  |  |  | +20 dBm    |
| 40 to 50 GHz      |  |  | +22 dBm    |
| 50 to 67 GHz      |  |  | +24 dBm    |

| <b>Third Order Intercept<sup>10</sup> - Tone spacing from 20 MHz - 50 MHz</b> |                        |                      |                   |
|-------------------------------------------------------------------------------|------------------------|----------------------|-------------------|
|                                                                               |                        |                      | <b>Any Option</b> |
|                                                                               |                        |                      | <b>typical</b>    |
| 10 MHz to 500 MHz                                                             |                        |                      | NA                |
| 500 MHz to 24 GHz                                                             |                        |                      | +26 dBm           |
| 24 to 40 GHz                                                                  |                        |                      | +24 dBm           |
| 40 to 50 GHz                                                                  |                        |                      | +25 dBm           |
| 50 to 67 GHz                                                                  |                        |                      | +27 dBm           |
| <b>Trace Noise Magnitude</b>                                                  |                        |                      |                   |
| 1 kHz IF bandwidth. Ratio measurement, nominal power at test port.            |                        |                      |                   |
|                                                                               | <b>Standard or 014</b> | <b>014 &amp; UNL</b> |                   |
| 10 MHz to 45 MHz <sup>2</sup>                                                 | <0.150 dB rms          | <0.150 dB rms        |                   |
| 45 MHz to 500 MHz <sup>11, 4</sup>                                            | <0.010 dB rms          | <0.010 dB rms        |                   |
| 500 MHz to 24 GHz                                                             | <0.006 dB rms          | <0.006 dB rms        |                   |
| 24 GHz to 67 GHz                                                              | <0.006 dB rms          | <0.009 dB rms        |                   |
| 67 GHz to 70 GHz <sup>2</sup>                                                 | <0.006 dB rms          | <0.009 dB rms        |                   |
| <b>Trace Noise Magnitude - Option 080 enabled<sup>2,5</sup></b>               |                        |                      |                   |
| 1 kHz IF bandwidth. Ratio measurement, nominal power at test port.            |                        |                      |                   |
|                                                                               | <b>Standard or 014</b> | <b>014 &amp; UNL</b> |                   |
|                                                                               |                        |                      |                   |
| 10 MHz to 45 MHz                                                              | <0.150 dB rms          | <0.150 dB rms        |                   |
| 45 MHz to 500 MHz <sup>11, 4</sup>                                            | <0.010 dB rms          | <0.010 dB rms        |                   |

|                                                                                                                                    |                   |               |                 |
|------------------------------------------------------------------------------------------------------------------------------------|-------------------|---------------|-----------------|
| 500 MHz to<br>24 GHz                                                                                                               | <0.006 dB rms     | <0.006 dB rms |                 |
| 24 GHz to<br>67 GHz                                                                                                                | <0.009 dB rms     | <0.012 dB rms |                 |
| 67 GHz to<br>70 GHz                                                                                                                | <0.009 dB rms     | <0.012 dB rms |                 |
| <b>Trace Noise Phase</b><br>1 kHz IF bandwidth. Ratio measurement, nominal power at test port.                                     |                   |               |                 |
|                                                                                                                                    | <b>Any Option</b> |               |                 |
| 10 MHz to<br>45 MHz <sup>2</sup>                                                                                                   | <0.800° rms       |               |                 |
| 45 MHz to<br>500 MHz <sup>4</sup>                                                                                                  | <0.100° rms       |               |                 |
| 500 MHz to<br>24 GHz                                                                                                               | <0.060° rms       |               |                 |
| 24 GHz to<br>67 GHz                                                                                                                | <0.100° rms       |               |                 |
| 67 GHz to<br>70 GHz <sup>2</sup>                                                                                                   | <0.100° rms       |               |                 |
| <b>Trace Noise Phase - Option 080 enabled<sup>2, 5</sup></b><br>1 kHz IF bandwidth. Ratio measurement, nominal power at test port. |                   |               |                 |
|                                                                                                                                    |                   |               | <b>typical:</b> |
| 10 MHz to<br>45 MHz                                                                                                                |                   |               | <0.800° rms     |
| 45 MHz to<br>500 MHz <sup>4</sup>                                                                                                  |                   |               | <0.100° rms     |
| 500 MHz to<br>24 GHz                                                                                                               |                   |               | <0.060° rms     |
| 24 GHz to<br>67 GHz                                                                                                                |                   |               | <0.100° rms     |
| 67 GHz to<br>70 GHz                                                                                                                |                   |               | <0.100° rms     |

| Reference Level Magnitude                                    |           |  |                   |
|--------------------------------------------------------------|-----------|--|-------------------|
| Range                                                        | +/-500 dB |  |                   |
| Resolution                                                   | 0.001 dB  |  |                   |
| Reference Level Phase                                        |           |  |                   |
| Range                                                        | +/-500°   |  |                   |
| Resolution                                                   | 0.01°     |  |                   |
| Stability Magnitude <sup>12</sup>                            |           |  |                   |
|                                                              |           |  | <b>Any Option</b> |
| <b>Typical</b> ratio measurement, made at the test port.     |           |  |                   |
| 10 MHz to<br>45 MHz                                          |           |  | +/-0.05 dB/°C     |
| 45 MHz to 50 GHz                                             |           |  | +/-0.02 dB/°C     |
| 50 GHz to<br>70 GHz                                          |           |  | +/-0.04 dB/°C     |
| Stability Phase <sup>12</sup>                                |           |  |                   |
|                                                              |           |  | <b>Any Option</b> |
| <b>Typical</b> ratio measurement, measured at the test port. |           |  |                   |
| 10 MHz to<br>45 MHz                                          |           |  | +/-0.5°/°C        |
| 45 MHz to<br>20 GHz                                          |           |  | +/-0.2°/°C        |
| 20 GHz to<br>40 GHz                                          |           |  | +/-0.5°/°C        |
| 40 GHz to<br>70 GHz                                          |           |  | +/-0.8°/°C        |
| Damage Input Level                                           |           |  |                   |
|                                                              |           |  |                   |
|                                                              |           |  | <b>typical:</b>   |

|                                        |  |  |                      |
|----------------------------------------|--|--|----------------------|
| Test Port 1 and 2                      |  |  | +27 dBm or +/-40 VDC |
| R1, R2 in                              |  |  | +15 dBm or +/-15 VDC |
| A, B in                                |  |  | +15 dBm or +/-7 VDC  |
| Coupler Thru (Option 014 or 014 & UNL) |  |  | +27 dBm or +/-40 VDC |
| Coupler Arm (Option 014 or 014 & UNL)  |  |  | +30 dBm or +/-7 VDC  |

1 Total average (rms) noise power calculated as the mean value of a linear magnitude trace expressed in dBm.

2 Typical performance.

3 Noise floor may be degraded by 10 dB at particular frequencies (multiples of 5 MHz) due to spurious receiver residuals.

4 Specified value is for worst-case noise floor at 45 MHz

50 Hz offset

6 Coupler roll-off will reduce compression below 500 MHz. Ultimately, at 45 MHz, compression is negligible.

7 Specified value is for worst-case compression at 500 MHz.

8 This compression level comes from the dynamic accuracy curve with -30 dBm reference test port power.

9 Option 016 degrades performance by 3 dB.

10 TOI is a typical specification that applies while the network analyzer receiver is in its linear range.

11 Trace noise magnitude may be degraded to 20 mdB rms at harmonic frequencies of the first IF (8.33 MHz) below 80 MHz.

12 Stability is defined as a ratio measurement made at the test port.


### Table 13. Dynamic Accuracy (Specification<sup>a</sup>)

Accuracy of the test port input power reading relative to the reference input power level.


**Note: If power is set above the maximum specified leveled power, the test port output signal may show non-linear effects that are dependent on the DUT**

#### Dynamic Accuracy, 0.045 GHz

## Magnitude

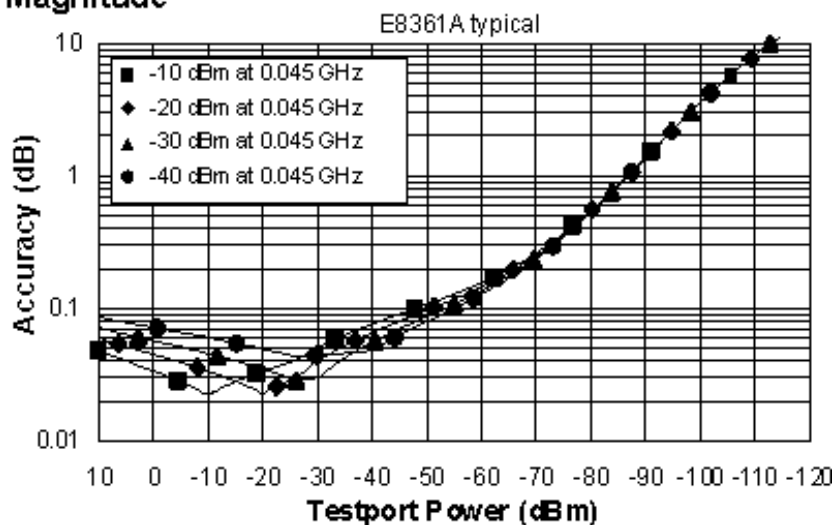


## Phase

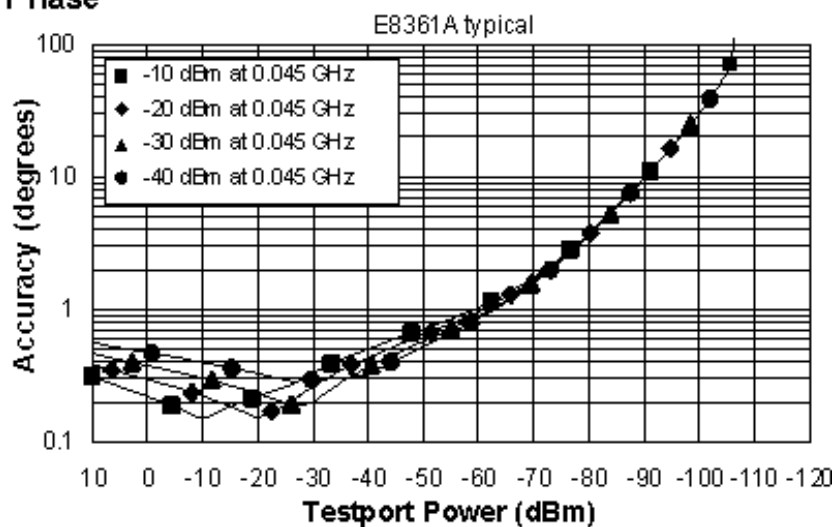


## Dynamic Accuracy, 0.500 GHz


## Magnitude

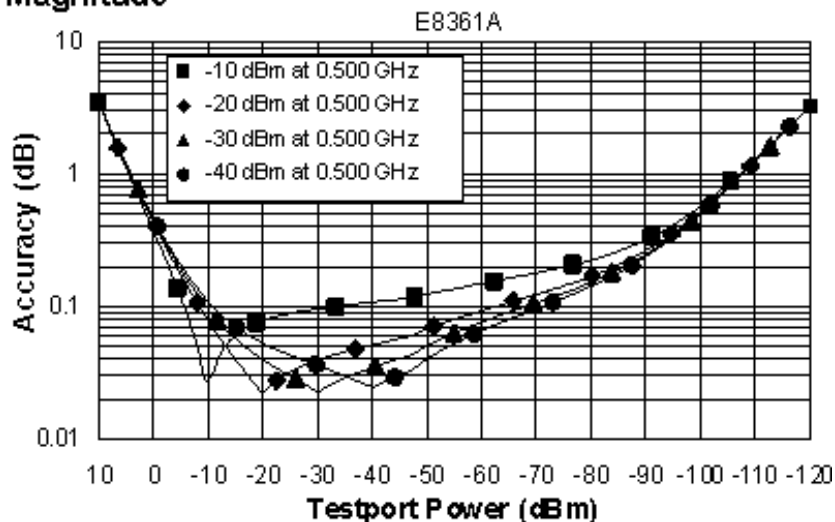


### Phase

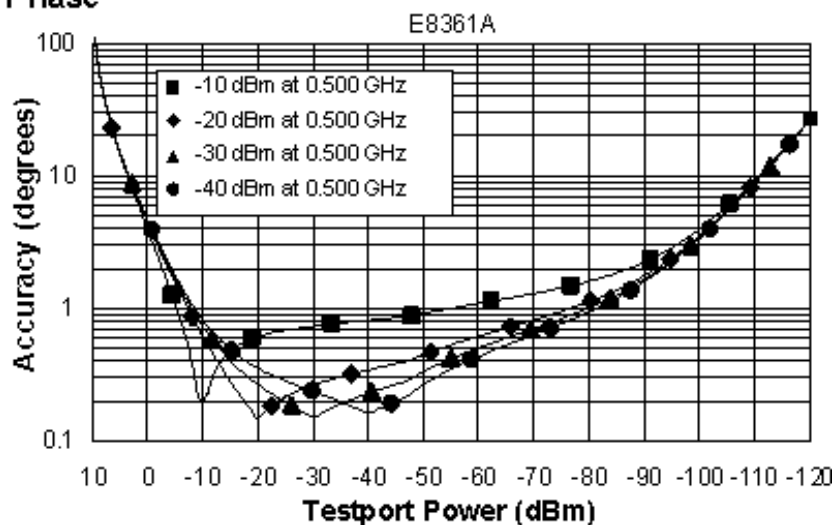

### Magnitude

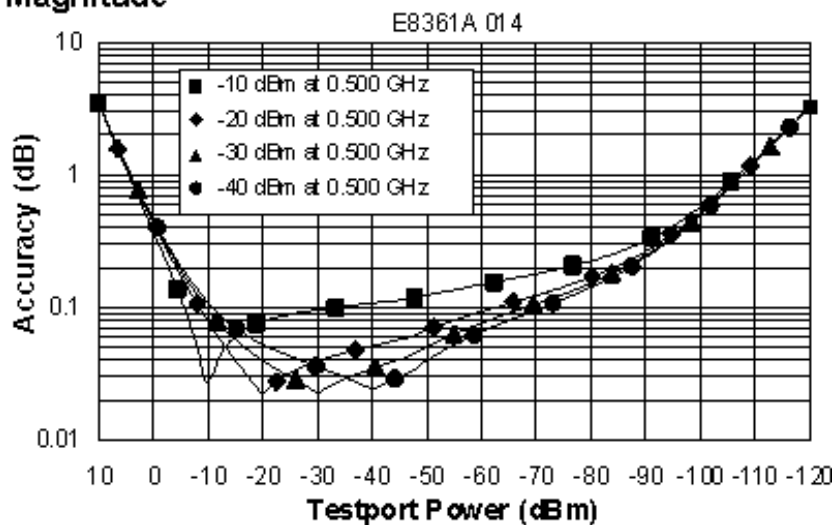


### Phase

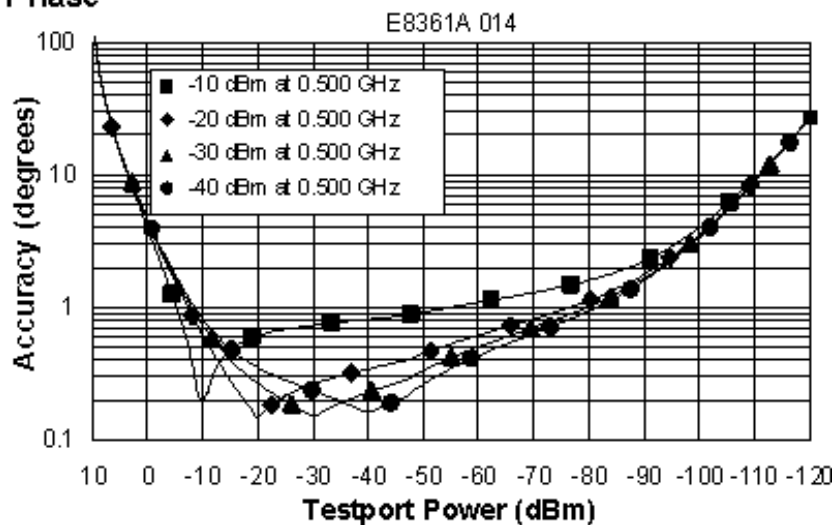





### Magnitude

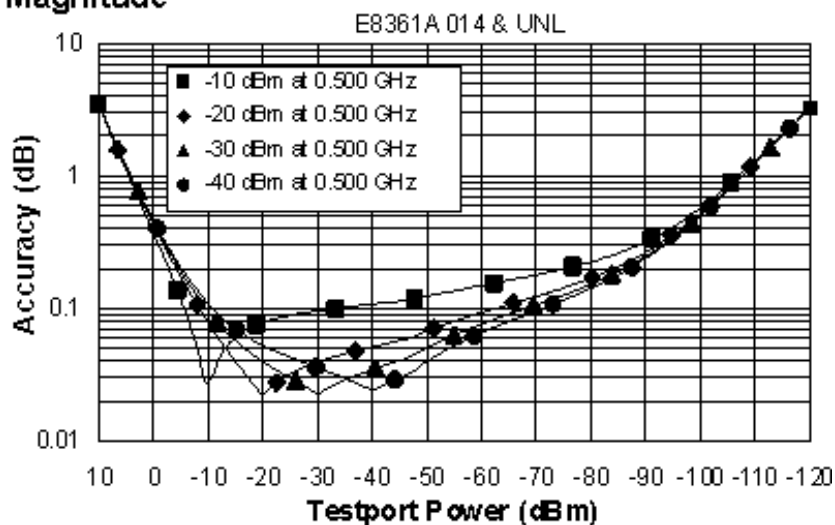


### Phase

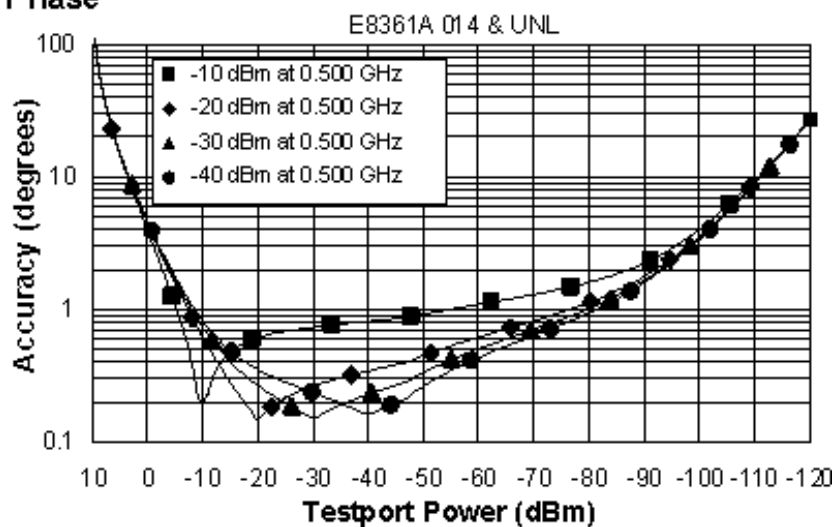

### Magnitude

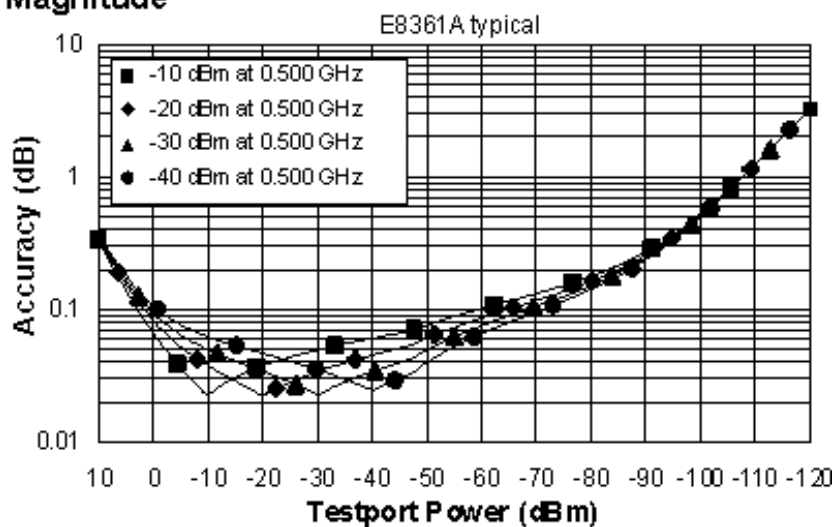


## Phase

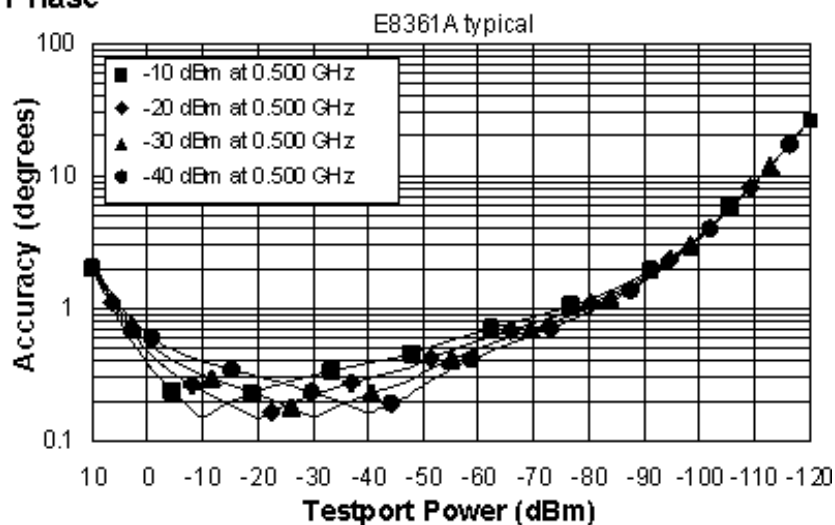


## Dynamic Accuracy, 0.500 - 5 GHz


### Magnitude

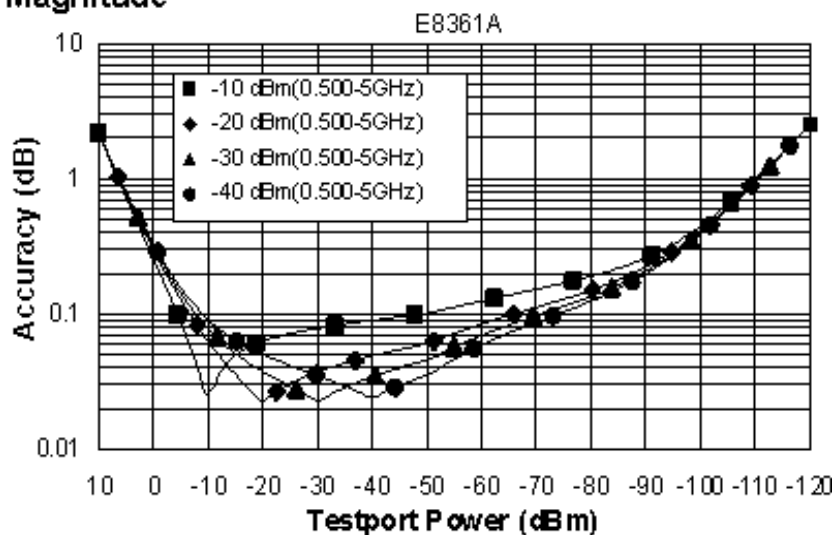


### Phase

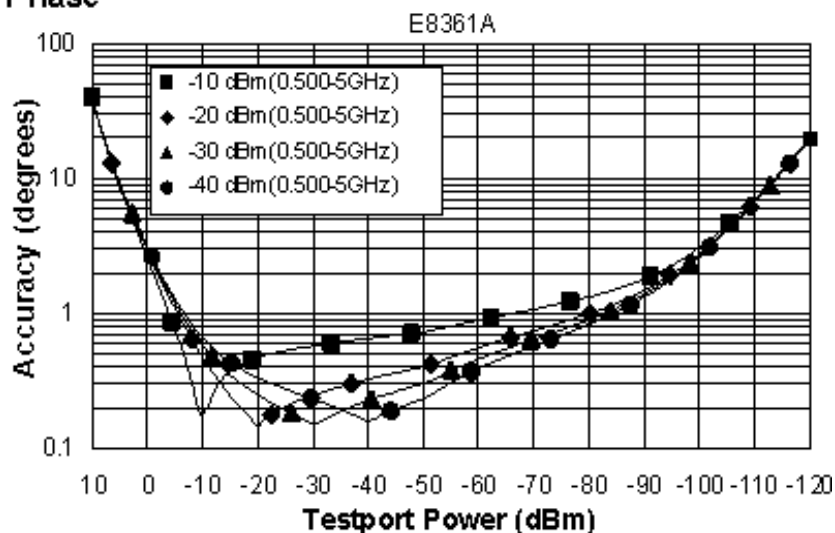


### Magnitude

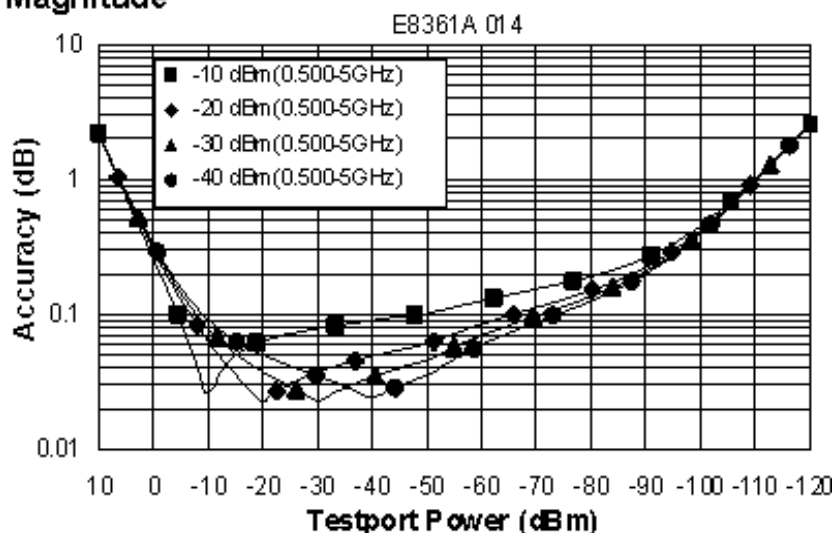


### Phase

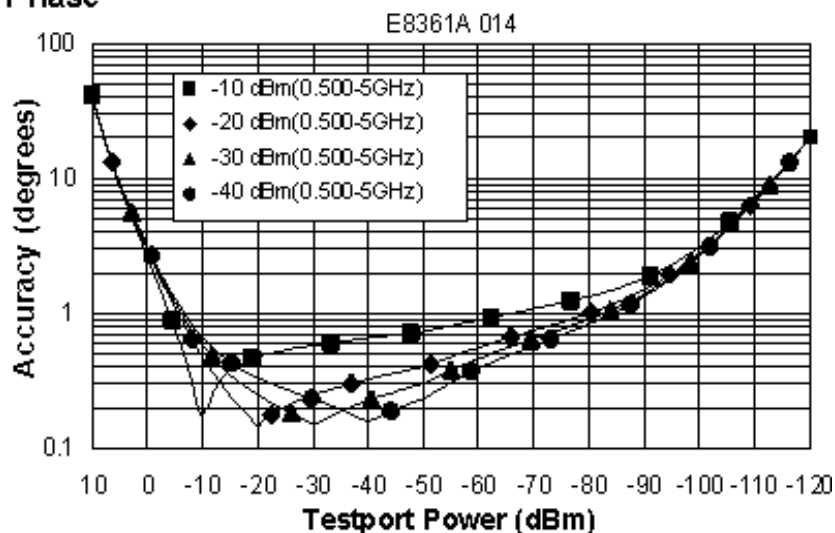


### Magnitude

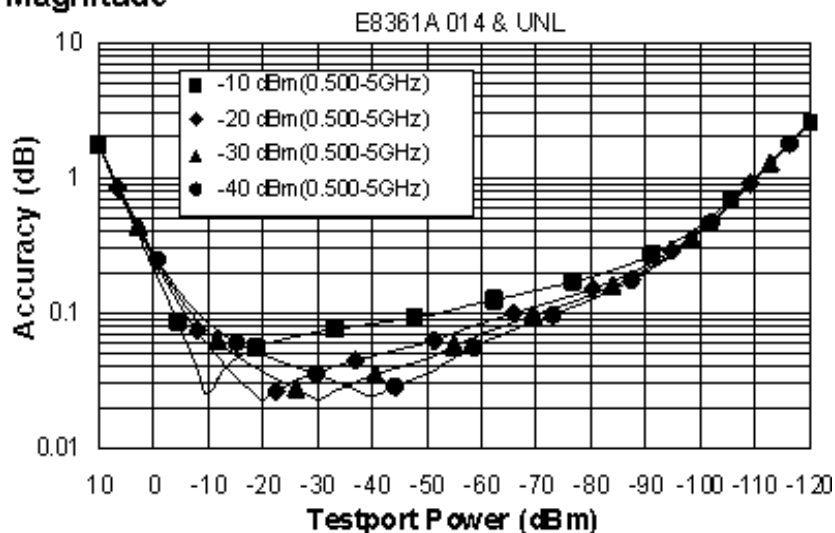


### Phase

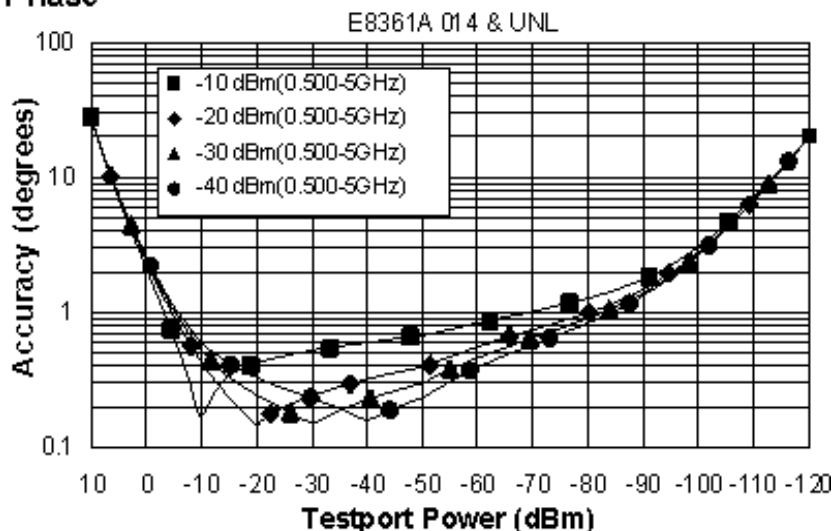

### Magnitude

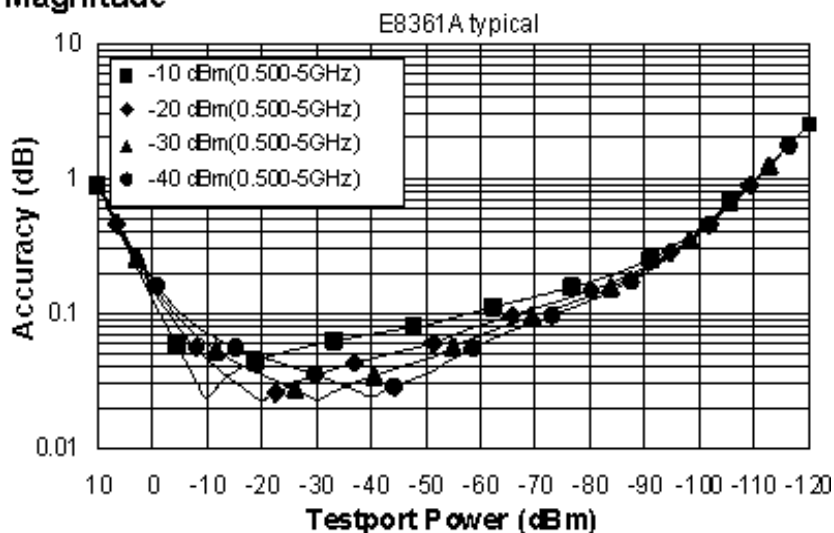


### Phase

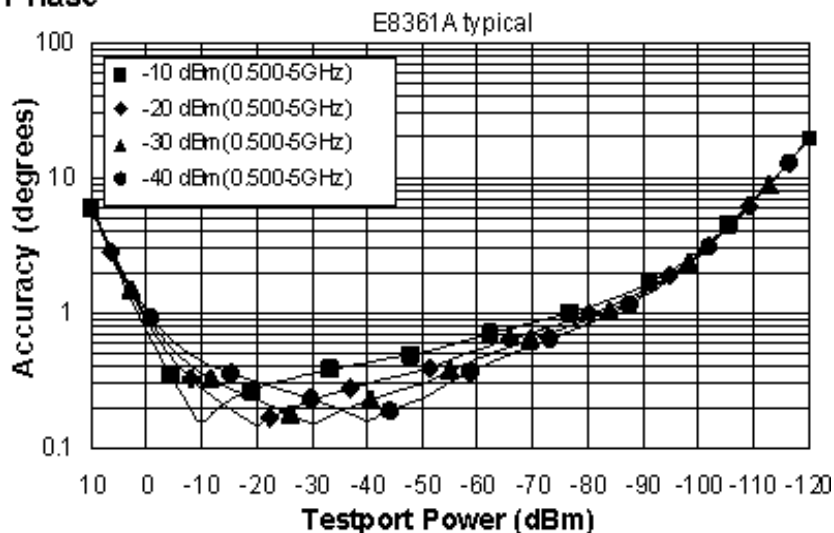


### Dynamic Accuracy, 5 - 30 GHz


### Magnitude

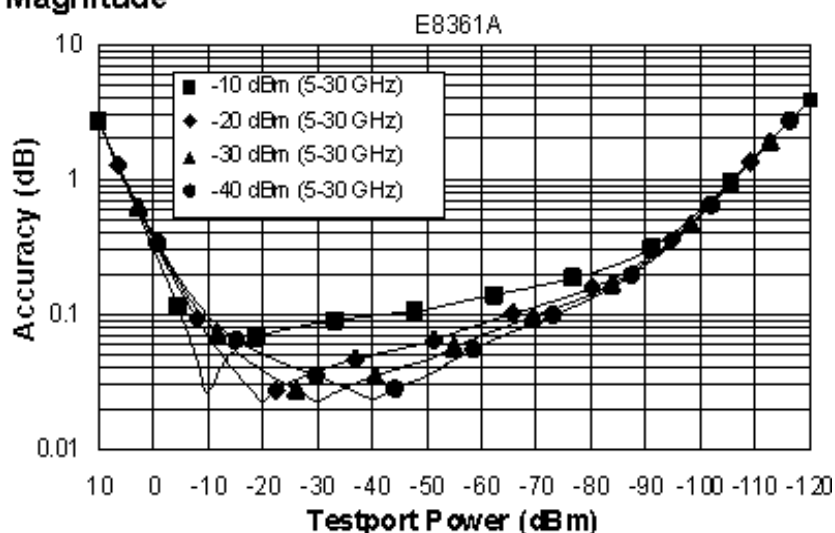


### Phase

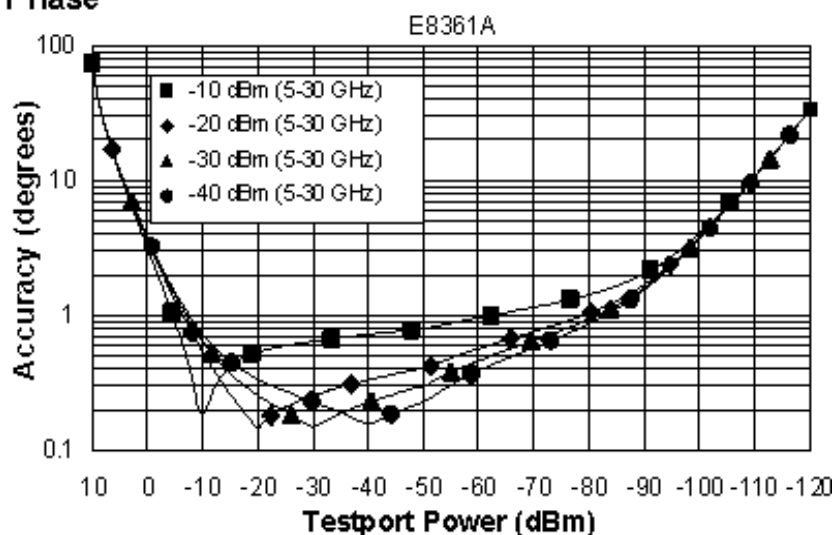


### Magnitude

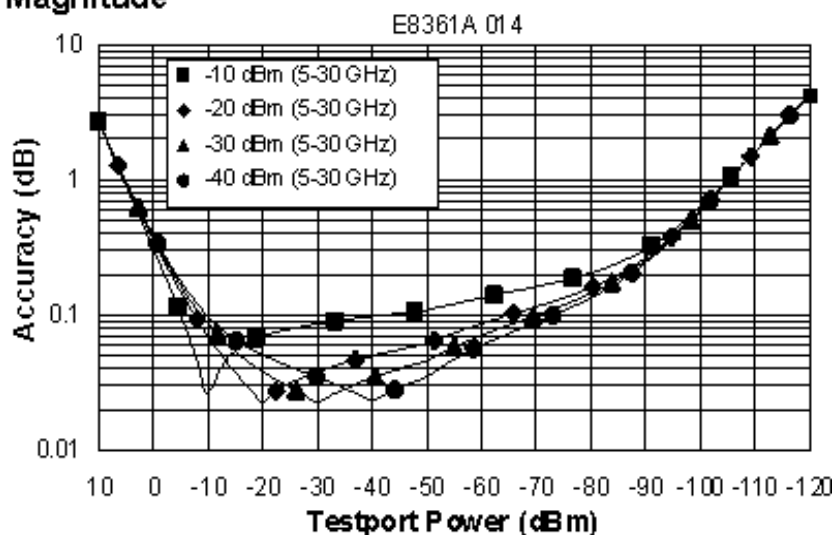


### Phase

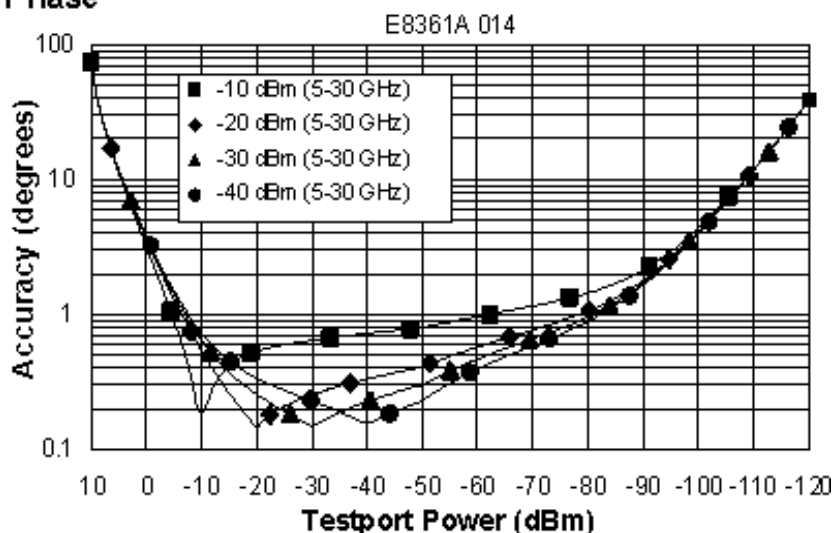


### Magnitude

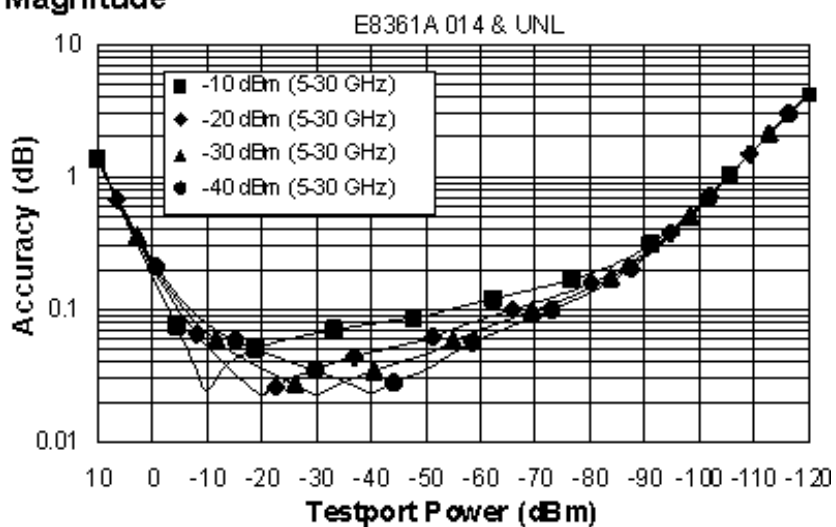


### Phase

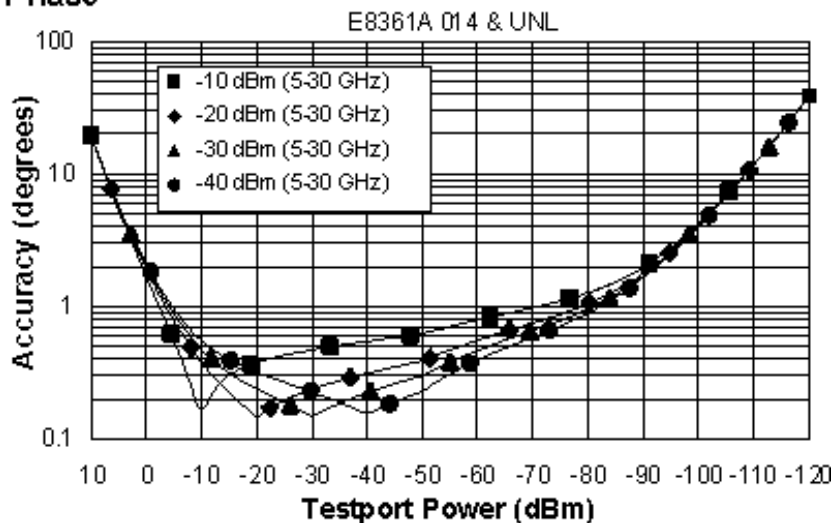

## Magnitude

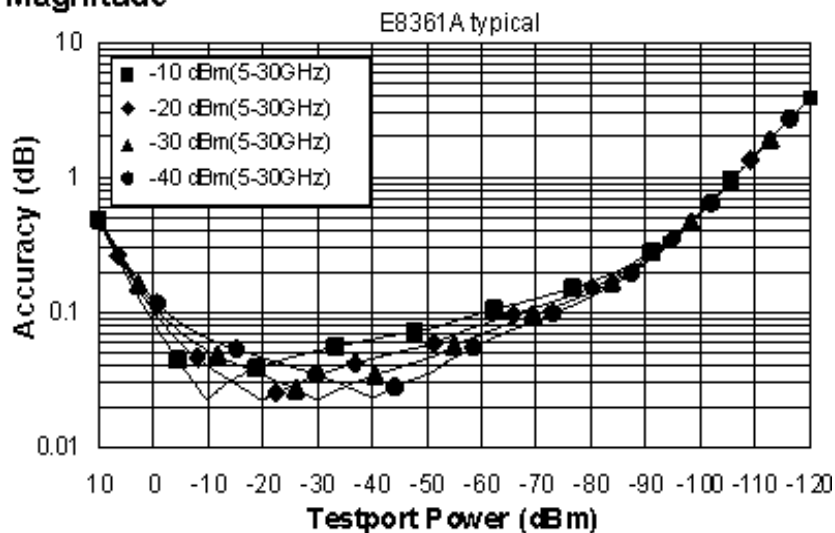


## Phase

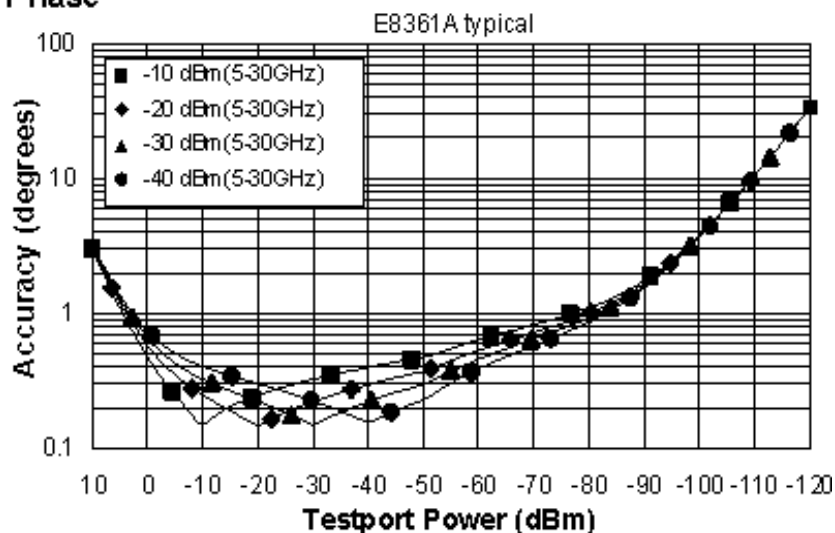


## Dynamic Accuracy, 30 - 67 GHz


### Magnitude

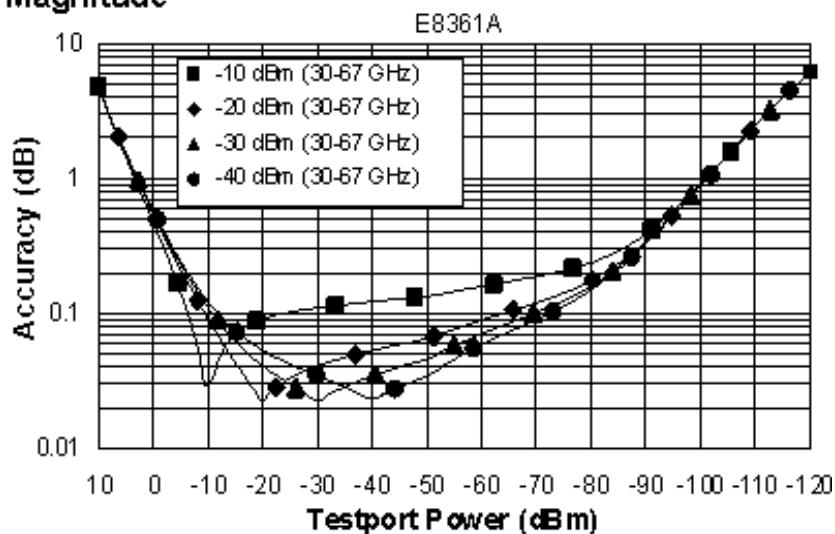


### Phase

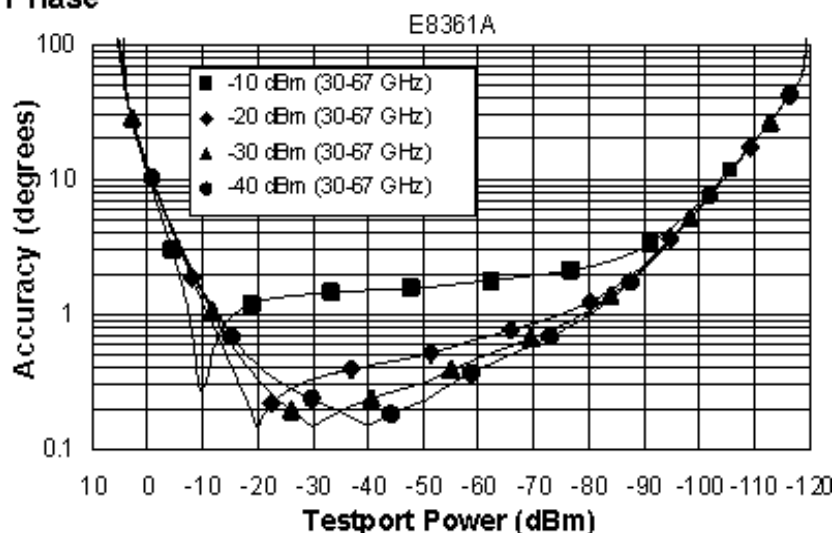

### Magnitude

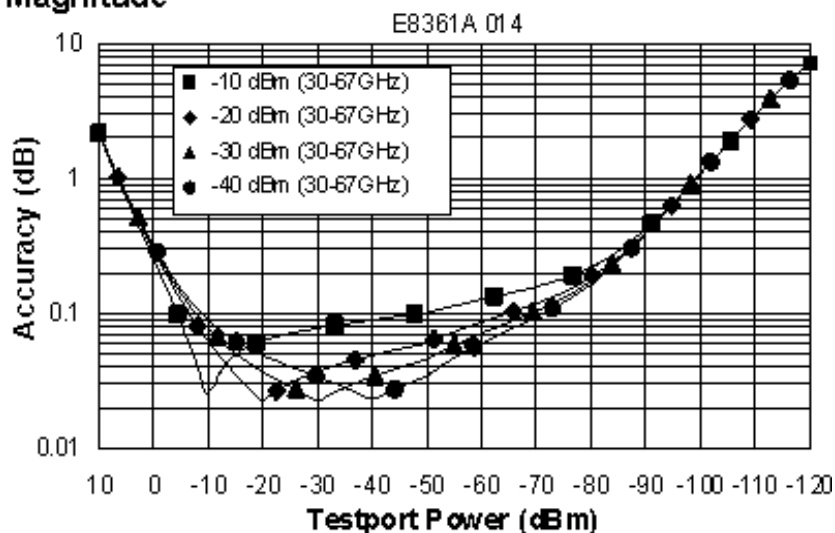


### Phase

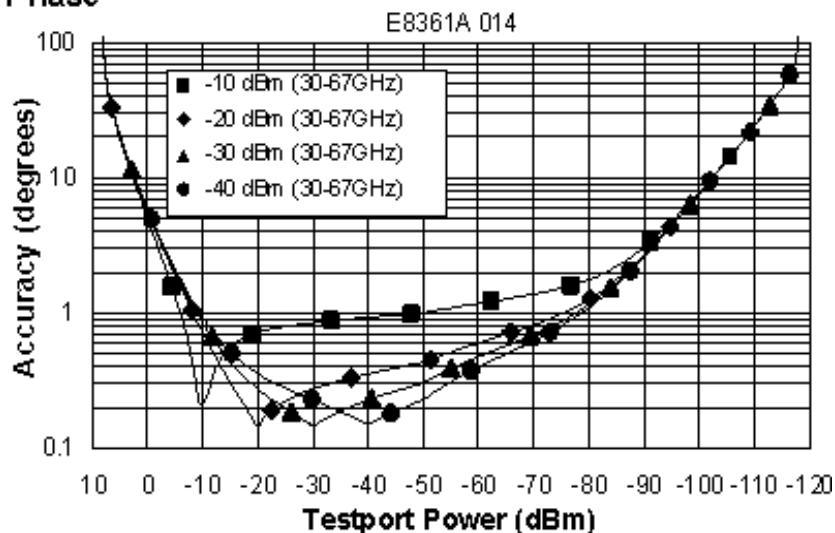





### Magnitude

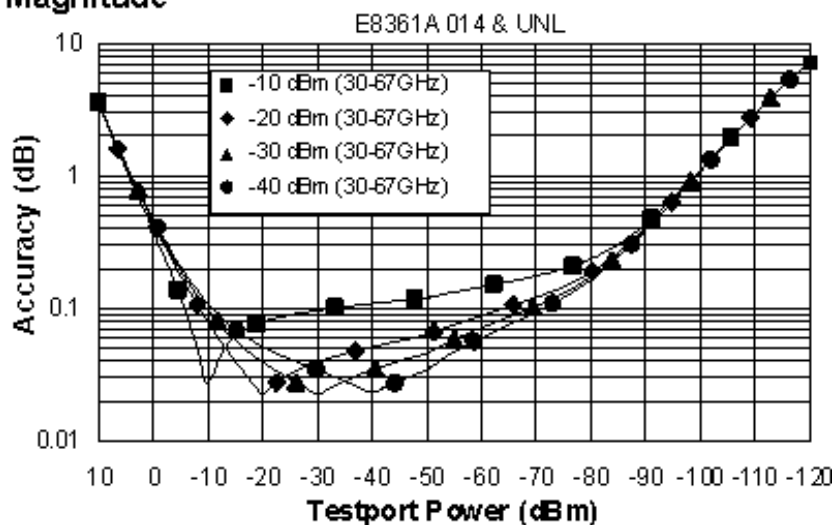


### Phase

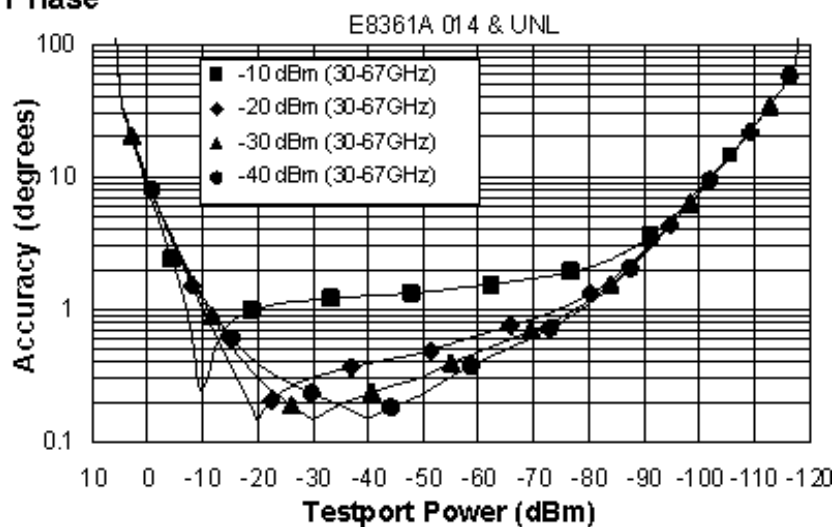

### Magnitude

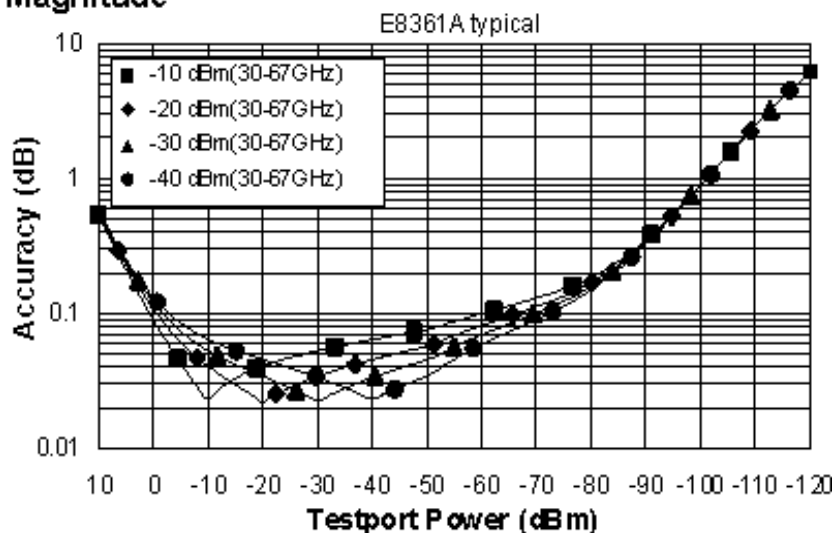


### Phase

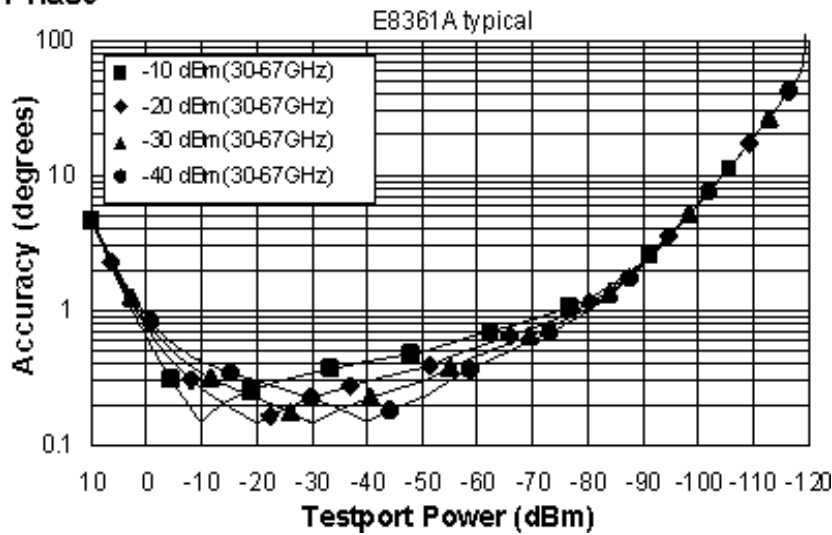


### Dynamic Accuracy, 67 - 70 GHz

#### Magnitude

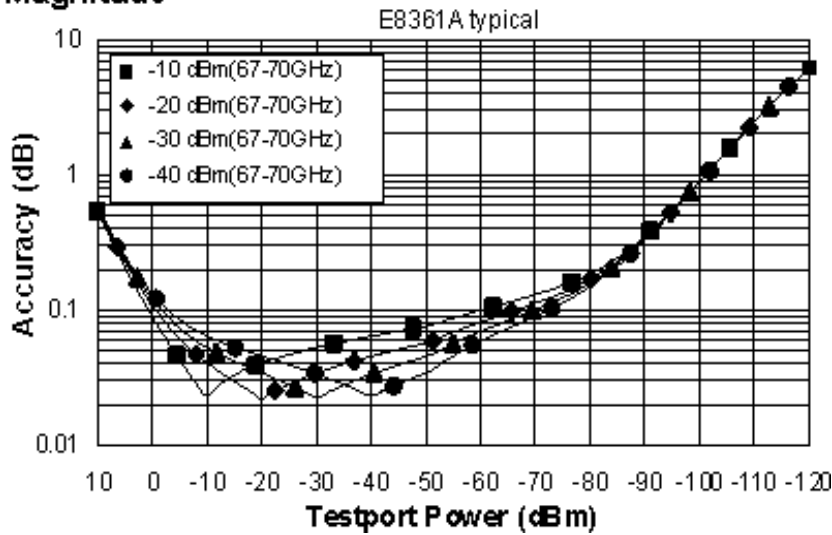

#### Phase

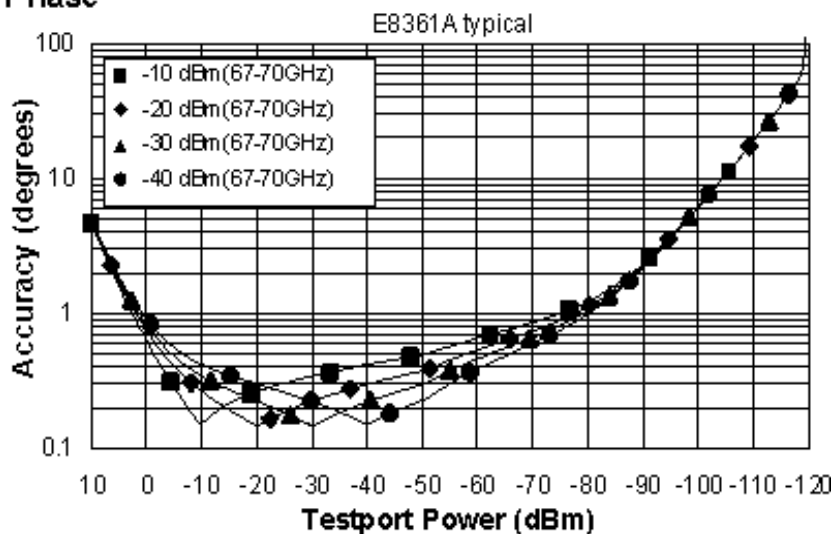


<sup>a</sup> Dynamic accuracy is verified with the following measurements:

- compression over frequency
- IF linearity at a single frequency of 1.195 GHz and a reference level of -20 dBm for an input power range of 0 to -120 dBm.

**Table 14. Test Port Input (Group Delay)<sup>a</sup>**

| Description           | Specification | Supplemental Information (typ.)                                                      |
|-----------------------|---------------|--------------------------------------------------------------------------------------|
| Aperture (selectable) |               | (frequency span)/(number of points -1)                                               |
| Maximum Aperture      |               | 20% of frequency span                                                                |
| Range                 |               | 0.5 x (1/minimum aperture)                                                           |
| Maximum Delay         |               | Limited to measuring no more than 180° of phase change within the minimum aperture.) |
| Accuracy              |               | See graph below. Char.                                                               |

The following graph shows characteristic group delay accuracy with full 2-port calibration and a 10 Hz IF bandwidth. Insertion loss is assumed to be < 2 dB and electrical length to be ten meters.

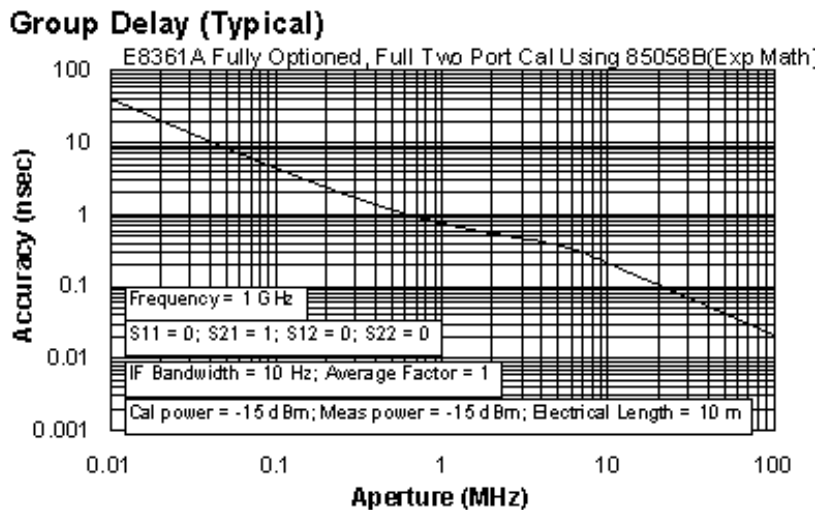

In general, the following formula can be used to determine the accuracy, in seconds, of specific group delay measurement:

$$\pm \text{Phase Accuracy (deg)} / [360 \times \text{Aperture (Hz)}]$$

Depending on the aperture and device length, the phase accuracy used is either incremental phase accuracy or worst case phase accuracy.

<sup>a</sup> Group delay is computed by measuring the phase change within a specified frequency step (determined by the frequency span and the number of points per sweep).

## General Information

### Miscellaneous Information

#### Front Panel

#### Rear Panel

#### Environment and Dimensions

**Table 15.** Miscellaneous Information

| Description               | Specification | Supplemental Information    |
|---------------------------|---------------|-----------------------------|
| System IF Bandwidth Range |               | 1 Hz to 40 kHz, nominal     |
| CPU                       |               | Intel® 500 MHz Pentium® III |

**Table 16.** Front Panel Information

| Description               | Supplemental Information                                                                        |
|---------------------------|-------------------------------------------------------------------------------------------------|
| <b>RF Connectors</b>      |                                                                                                 |
| <b>E8361A</b>             |                                                                                                 |
| Type                      | 1.85 mm (male), 50 ohm, (nominal)                                                               |
| Center Pin Recession      | 0.002 in. (characteristic)                                                                      |
| <b>Display</b>            |                                                                                                 |
| Size                      | 21.3 cm (8.4 in) diagonal color active matrix LCD; 640 (horizontal) X 480 (vertical) resolution |
| Refresh Rate              | Vertical 59.83 Hz; Horizontal 31.41 kHz                                                         |
| <b>Display Range</b>      |                                                                                                 |
| Magnitude                 | ±200 dB (at 20 dB/div), max                                                                     |
| Phase                     | ±500°, max                                                                                      |
| Polar                     | 10 pUnits, min<br>1000 Units, max                                                               |
| <b>Display Resolution</b> |                                                                                                 |
| Magnitude                 | 0.001 dB/div, min                                                                               |
| Phase                     | 0.01°/div, min                                                                                  |
| <b>Marker Resolution</b>  |                                                                                                 |
| Magnitude                 | 0.001 dB, min                                                                                   |
| Phase                     | 0.01°, min                                                                                      |
| Polar                     | 0.01 mUnit, min; 0.01°,min                                                                      |

**Table 17.** Rear Panel Information

| Description                | Supplemental Information    |
|----------------------------|-----------------------------|
| <b>10 MHz Reference In</b> |                             |
| Connector                  | BNC, female                 |
| Input Frequency            | 10 MHz ± 10 ppm, typical    |
| Input Level                | -15 dBm to +20 dBm, typical |

|                                                             |                                                                                |
|-------------------------------------------------------------|--------------------------------------------------------------------------------|
| Input Impedance                                             | 200 $\Omega$ , nom.                                                            |
| <b>10 MHz Reference Out</b>                                 |                                                                                |
| Connector                                                   | BNC, female                                                                    |
| Output Frequency                                            | 10 MHz $\pm$ 1 ppm, typical                                                    |
| Signal Type                                                 | Sine Wave, typical                                                             |
| Output Level                                                | +10 dBm $\pm$ 4 dB into 50 $\Omega$ , typical                                  |
| Output Impedance                                            | 50 $\Omega$ , nominal                                                          |
| Harmonics                                                   | <-40 dBc, typical                                                              |
| <b>Option H08 &amp; H11 Rear Panel Connectors (Typical)</b> |                                                                                |
| IF Connectors                                               | A, R1, R2, B (BNC Connectors)                                                  |
| IF Connector Input Frequency                                | 8 1/3 MHz                                                                      |
| Nominal Input Impedance at IF Inputs                        | 50 $\Omega$                                                                    |
| RF Damage Level to IF Connector Inputs                      | -20.0 dBm                                                                      |
| DC Damage Level to IF Connector Inputs                      | 25 volts                                                                       |
| 0.1 dB Compression Point at IF Inputs                       | -27.0 dBm                                                                      |
| Pulse Input Connectors <sup>1</sup>                         | A, R1, R2, B (BNC Connectors)                                                  |
| Nominal Input Impedance at Pulse Inputs                     | 1 Kohm                                                                         |
| Minimum IF Gate Width                                       | 20 ns for less than 1 dB deviation from theoretical performance <sup>2</sup> . |
| DC Damage Level to Pulse Connector Inputs                   | 5.5 volts                                                                      |
| Drive Voltage                                               | TTL (0, +5.0) Volts                                                            |
| <b>Rear Panel LO Power - Test Port Frequency</b>            |                                                                                |
| 1.7 GHz to 20 GHz                                           | -7 to -16 dBm                                                                  |
| <b>Rear Panel RF Power - Test Port Frequencies</b>          |                                                                                |
| 1.7 GHz to 20 GHz                                           | -2 to -12 dBm (at -5 dBm test port power <sup>3</sup> )                        |

|                                           |                                                                                                                                                                                                                    |
|-------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 10 GHz to 16 GHz                          | 0 to -8 dBm (at -5 dBm test port power <sup>3</sup> )                                                                                                                                                              |
| 16 GHz to 20 GHz                          | +5 to -1 dBm (at -5 dBm test port power <sup>3</sup> )                                                                                                                                                             |
| <b>VGA Video Output</b>                   |                                                                                                                                                                                                                    |
| Connector                                 | 15-pin mini D-Sub; Drives VGA compatible monitors                                                                                                                                                                  |
| Devices Supported:                        |                                                                                                                                                                                                                    |
|                                           | <b>Resolutions:</b>                                                                                                                                                                                                |
| Flat Panel (TFT)                          | 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                                   |
| Flat Panel (DSTN)                         | 800 X 600, 640 X 480                                                                                                                                                                                               |
| CRT Monitor                               | 1280 X 1024, 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                      |
|                                           | Simultaneous operation of the internal and external displays is allowed, but with 640 X 480 resolution only. If you change resolution, you can only view the external display (internal display will "white out"). |
| <b>Bias Input Connectors (Option UNL)</b> |                                                                                                                                                                                                                    |
| Bias current                              | 500 mA, maximum                                                                                                                                                                                                    |
| Bias voltage                              | 40 Volts, maximum                                                                                                                                                                                                  |
| <b>Test Set IO</b>                        |                                                                                                                                                                                                                    |
|                                           | 25-pin D-Sub connector, available for external test set control                                                                                                                                                    |
| <b>Aux IO</b>                             |                                                                                                                                                                                                                    |
|                                           | 25-pin D-Sub connector, male, analog and digital IO                                                                                                                                                                |
| <b>Handler IO</b>                         |                                                                                                                                                                                                                    |
|                                           | 36-pin parallel I/O port; all input/output signals are default set to negative logic; can be reset to positive logic via GPIB command                                                                              |
| <b>GPIB</b>                               |                                                                                                                                                                                                                    |
|                                           | 24-pin D-sub (Type D-24), female; compatible with IEEE-488.                                                                                                                                                        |
| <b>Parallel Port (LPT1)</b>               |                                                                                                                                                                                                                    |
|                                           | 25-pin D-Sub miniature connector, female; provides connection to printers or any other parallel port peripherals                                                                                                   |
| <b>Serial Port (COM 1)</b>                |                                                                                                                                                                                                                    |
|                                           | 9-pin D-Sub, male; compatible with RS-232                                                                                                                                                                          |
| <b>USB Port</b>                           |                                                                                                                                                                                                                    |

|                               |                                                                                                                                                      |
|-------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------|
|                               | One port on front panel and five ports on rear panel. Universal Serial Bus jack, Type A configuration (4 contacts inline, contact 1 on left); female |
| Contact 1                     | Vcc: 4.75 to 5.25 VDC, 500 mA, maximum                                                                                                               |
| Contact 2                     | -Data                                                                                                                                                |
| Contact 3                     | +Data                                                                                                                                                |
| Contact 4                     | Ground                                                                                                                                               |
| <b>LAN</b>                    |                                                                                                                                                      |
|                               | 10/100BaseT Ethernet, 8-pin configuration; auto selects between the two data rates                                                                   |
| <b>Line Power<sup>4</sup></b> |                                                                                                                                                      |
| Frequency                     | 48 Hz to 66 Hz                                                                                                                                       |
| Voltage at 115 V Setting      | 90 to 132 VAC; 120 VAC, nominal                                                                                                                      |
| Voltage at 220 V Setting      | 198 to 264 VAC; 240 VAC, nominal                                                                                                                     |
| VA Max                        | 600 VA maximum                                                                                                                                       |

1 Pulse input connectors are operational only with Option H08 (Pulse Measurement Capability) enabled.

2 Based on deviation from signal reduction equation: Signal Reduction (dB) =  $20\log_{10}(\text{Duty\_cycle}) = 20\log_{10}(\text{pulse\_width/period})$ .  
Measured at Pulse Repetition Frequency (PFR) of 1 MHz.

3 Test port power has to be at a high enough level such that the "Drop Cal" does not occur. If Drop Cal occurs then the power out of the rear panel RF connector will drop by about 15 dB.

4 A third-wire ground is required.

**Table 18.** Analyzer Environment and Dimensions

| Description                       | Supplemental Information                                                                                                                                                                                                                                              |
|-----------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>General Environmental</b>      |                                                                                                                                                                                                                                                                       |
| RFI/EMI Susceptibility            | Defined by CISPR Pub. 11, Group 1, Class A, and IEC 50082-1                                                                                                                                                                                                           |
| ESD                               | Minimize using static-safe work procedures and an antistatic bench mat                                                                                                                                                                                                |
| Dust                              | Minimize for optimum reliability                                                                                                                                                                                                                                      |
| <b>Operating Environment</b>      |                                                                                                                                                                                                                                                                       |
| Temperature                       | 0 °C to +40 °C<br><br>Instrument powers up, phase locks, and displays no error messages within this temperature range (except for "source unleveled" error message that may occur at temperatures outside the specified performance temperature range of 25 +/- 5°C). |
| Error-Corrected Temperature Range | 23°C ± 3°C<br>with less than 1°C deviation from calibration temp.                                                                                                                                                                                                     |
| Humidity                          | 5% to 95% at +40 °C                                                                                                                                                                                                                                                   |

|                                          |                                      |
|------------------------------------------|--------------------------------------|
| Altitude                                 | 0 to 4500 m (14,760 ft.)             |
| <b>Non-Operating Storage Environment</b> |                                      |
| Temperature                              | -40 °C to +70 °C                     |
| Humidity                                 | 0% to 90% at +65 °C (non-condensing) |
| Altitude                                 | 0 to 15,240 m (50,000 ft.)           |

| <b>Cabinet Dimensions</b>                                                   |                          |                    |                    |
|-----------------------------------------------------------------------------|--------------------------|--------------------|--------------------|
|                                                                             | <b>Height</b>            | <b>Width</b>       | <b>Depth</b>       |
| Excluding front and rear panel hardware and feet                            | 267 mm<br>10.5 in        | 426 mm<br>16.75 in | 427 mm<br>16.8 in  |
| As shipped - includes front panel connectors, rear panel bumpers, and feet. | 280 mm<br>11.0 in        | 435 mm<br>17.1 in  | 470 mm<br>18.5 in  |
| As shipped plus handles                                                     | 280 mm<br>11.0 in        | 458 mm<br>18 in    | 501 mm<br>19.7 in  |
| As shipped plus rack-mount flanges                                          | 280 mm<br>11.0 in        | 483 mm<br>19 in    | 470 mm<br>18.5 in  |
| As shipped plus handles and rack-mount flanges                              | 280 mm<br>11.0 in        | 483 mm<br>19 in    | 501 mm<br>19.70 in |
| <b>Weight</b>                                                               |                          |                    |                    |
| <b>Net</b>                                                                  |                          |                    |                    |
| E8361A                                                                      | 29 kg (64 lb), nominal   |                    |                    |
| <b>Shipping</b>                                                             |                          |                    |                    |
| E8361A                                                                      | 36.3 kg (80 lb), nominal |                    |                    |

**Measurement Throughput Summary**

[Typical Cycle Time for Measurement Completion](#)

[Cycle Time vs IF Bandwidth](#)

[Cycle Time vs Number of Points](#)

[Data Transfer Time](#)

**Table 19** Typical Cycle Time<sup>a,b</sup> (ms) for Measurement Completion



|                                                       | Number of Points |     |      |        |
|-------------------------------------------------------|------------------|-----|------|--------|
|                                                       | 201              | 401 | 1601 | 16,001 |
| <b>Start 28 GHz, Stop 30 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 12               | 19  | 55   | 503    |
| 2-Port cal                                            | 29               | 44  | 124  | 1112   |
| <b>Start 10 MHz, Stop 10 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 86               | 93  | 121  | 583    |
| 2-Port cal                                            | 179              | 199 | 267  | 1301   |
| <b>Start 10 MHz, Stop 20 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 126              | 130 | 153  | 597    |
| 2-Port cal                                            | 264              | 275 | 335  | 1321   |
| <b>Start 10 MHz, Stop 40 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 185              | 190 | 213  | 621    |
| 2-Port cal                                            | 382              | 401 | 459  | 1374   |
| <b>Start 10 MHz, Stop 50 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 210              | 216 | 243  | 643    |
| 2-Port cal                                            | 436              | 450 | 522  | 1405   |
| <b>Start 10 MHz, Stop 67 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected<br>1-port cal                             | 244              | 254 | 300  | 645    |
| 2-Port cal                                            | 502              | 524 | 591  | 1423   |

a Typical performance.

b Includes sweep time, retrace time and band-crossing time. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S11) measurement.

**Table 20. Cycle Time vs IF Bandwidth<sup>a</sup>**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 28 GHz

- Span = 100 MHz
- Display off (add 21 ms for display on)

| IF Bandwidth (Hz) | Cycle Time (ms) <sup>b</sup> | Cycle Time (ms)<br>Option 080<br>enabled |
|-------------------|------------------------------|------------------------------------------|
| 40,000            | 11                           | 100                                      |
| 35,000            | 12                           | 101                                      |
| 30,000            | 13                           | 102                                      |
| 20,000            | 16                           | 106                                      |
| 10,000            | 30                           | 127                                      |
| 7000              | 38                           | 138                                      |
| 5000              | 50                           | 152                                      |
| 3000              | 74                           | 182                                      |
| 1000              | 274                          | 326                                      |
| 300               | 694                          | 782                                      |
| 100               | 1905                         | 2054                                     |
| 30                | 6091                         | 6355                                     |
| 10                | 17916                        | 18372                                    |

a Typical performance.

b Cycle time includes sweep and retrace time.

**Table 21. Cycle Time vs Number of Points<sup>a</sup>**

Applies to the Preset condition (35 kHz IF bandwidth, correction off) except for the following changes:

- CF = 28 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Number of Points | Cycle Time (ms) <sup>b</sup> |
|------------------|------------------------------|
| 3                | 6                            |
| 11               | 6                            |
| 51               | 7                            |
| 101              | 9                            |
| 201              | 12                           |
| 401              | 18                           |
| 801              | 30                           |
| 1601             | 55                           |
| 16,001           | 497                          |

a Typical performance.

b Cycle time includes sweep and retrace time.

**Table 22.** Data Transfer Time (ms)<sup>a</sup>


|                                                            | Number of Points |     |      |        |
|------------------------------------------------------------|------------------|-----|------|--------|
|                                                            | 201              | 401 | 1601 | 16,001 |
| <b>SCPI over GPIB</b><br>(program executed on external PC) |                  |     |      |        |
| 32-bit floating point                                      | 7                | 12  | 43   | 435    |
| 64-bit floating point                                      | 12               | 22  | 84   | 856    |
| ASCII                                                      | 64               | 124 | 489  | 5054   |
| <b>SCPI</b><br>(program executed in the analyzer)          |                  |     |      |        |
| 32-bit floating point                                      | 1                | 2   | 3    | 30     |
| 64-bit floating point                                      | 2                | 2   | 4    | 40     |
| ASCII                                                      | 29               | 56  | 222  | 2220   |
| <b>COM (program executed in the analyzer)</b>              |                  |     |      |        |
| 32-bit floating point                                      | <0.4             | 0.4 | 0.5  | 1.9    |
| Variant type                                               | 0.7              | 1   | 3    | 32     |
| <b>DCOM over LAN</b><br>(program executed on external PC)  |                  |     |      |        |
| 32-bit floating point                                      | <0.8             | 1   | 1.5  | 7.1    |
| Variant type                                               | 1.8              | 2.7 | 8.5  | 80     |

a Typical performance


**Note:** Specifications for Recall & Sweep Speed are not provided for the E8361A analyzers.

## Test Set Block Diagrams

E8361A - Standard Configuration and Standard Power Range

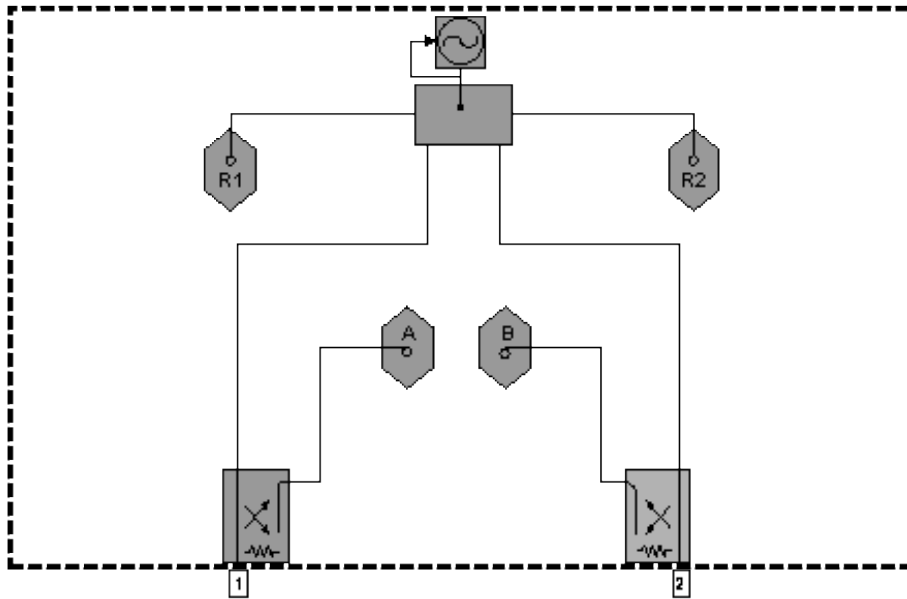


E8361A - Option UNL Standard Configuration with Extended Power Range and Bias - Tees

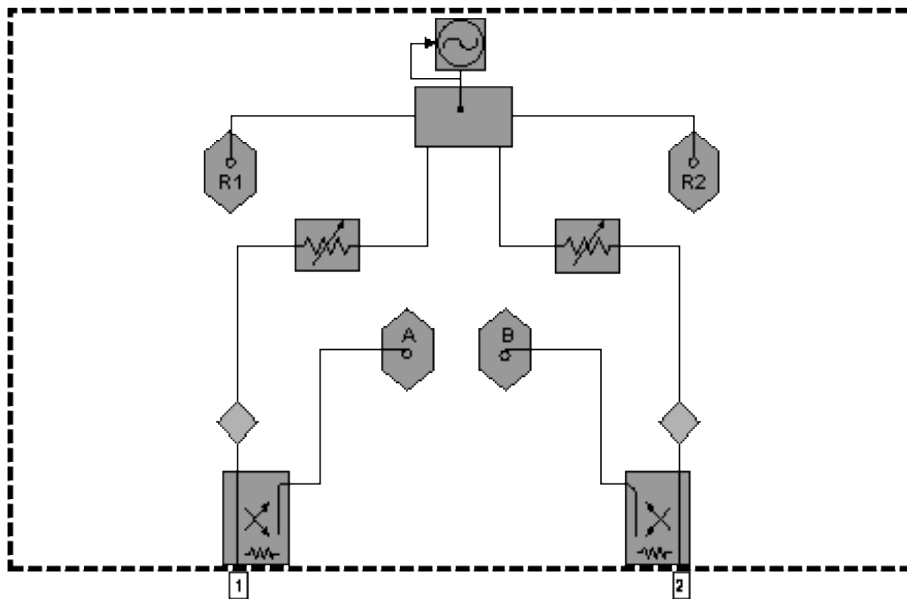


E8361A - Option UNL Standard Configuration with Extended Power Range and Bias - Tees, and Option 016,

## Receiver Attenuators

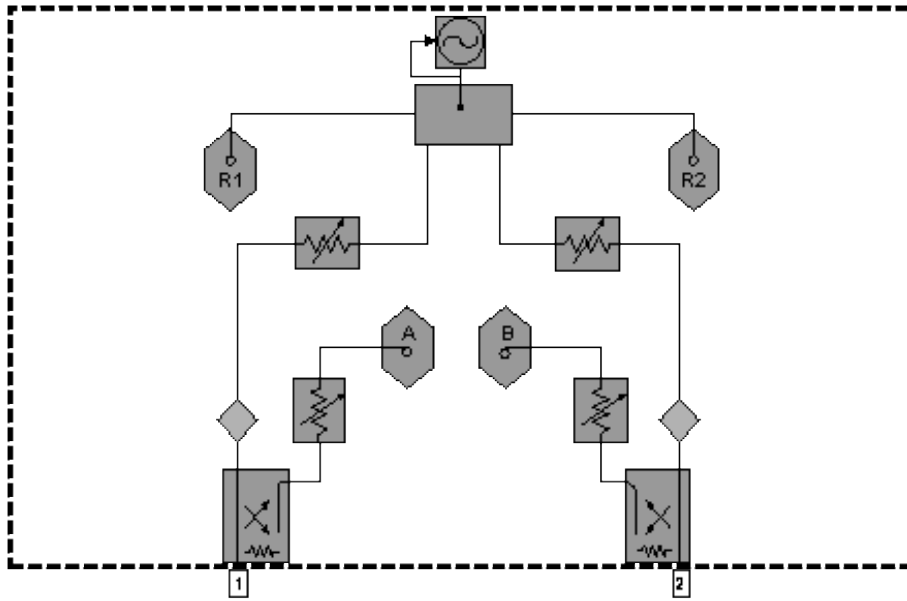


## Test Set with Option 014 Block Diagrams

E8361A - Option 014 – Configurable Test Set and Standard Power Range

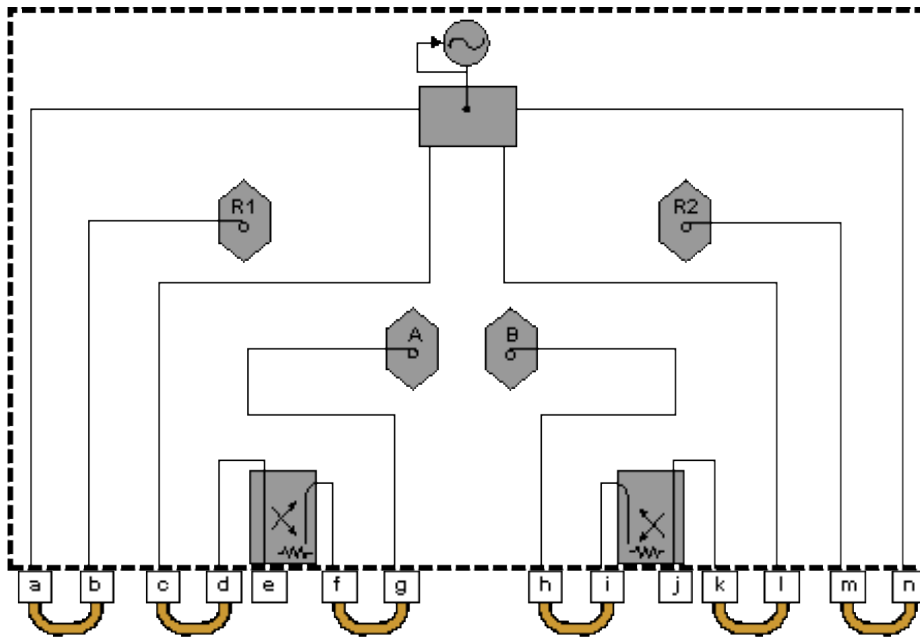


| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

E8361A - Option 014 – Configurable Test Set and Standard Power Range, and Option 081 Reference Channel Transfer Switch

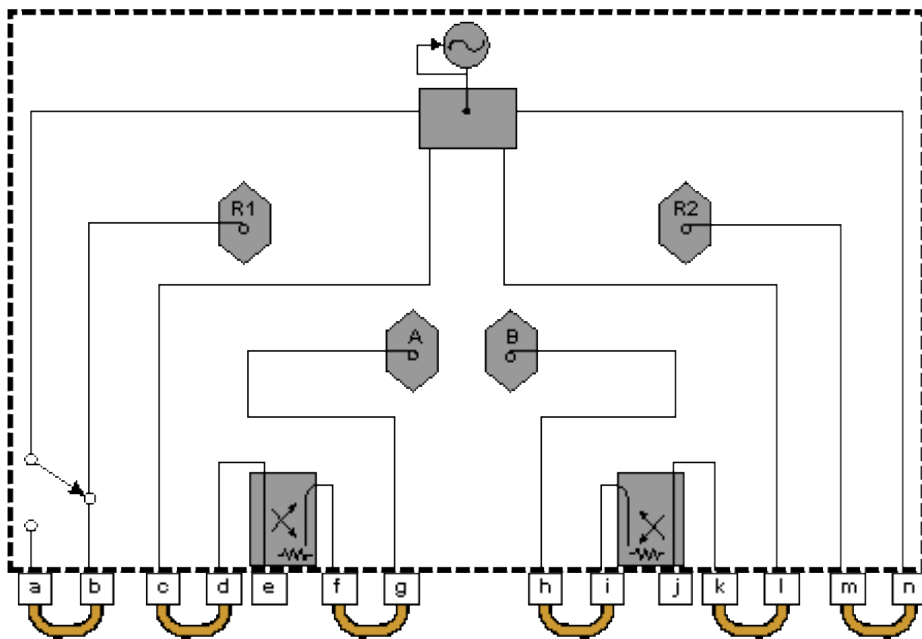


| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

E8361A - Option 014 Configurable Test Set, and Option UNL Extended Power Range and Bias - Tees

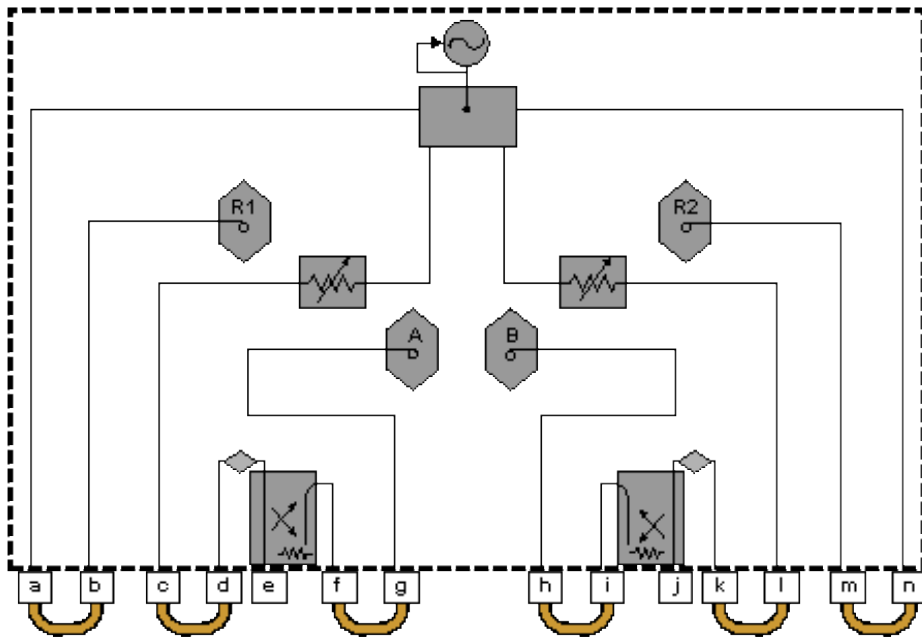

| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |


E8361A - Option 014 Configurable Test Set, and Option UNL Extended Power Range and Bias - Tees, and Option 081 Reference Channel Transfer Switch

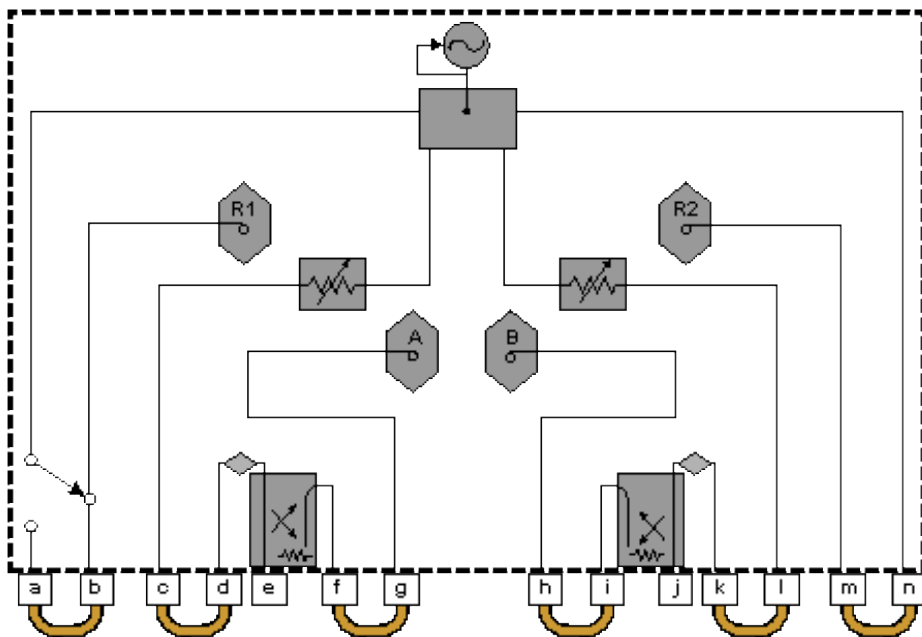




| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

E8361A - Option 014 Configurable Test Set and Option UNL, Extended Power Range and Bias - Tees and Option 016 Receiver Attenuators

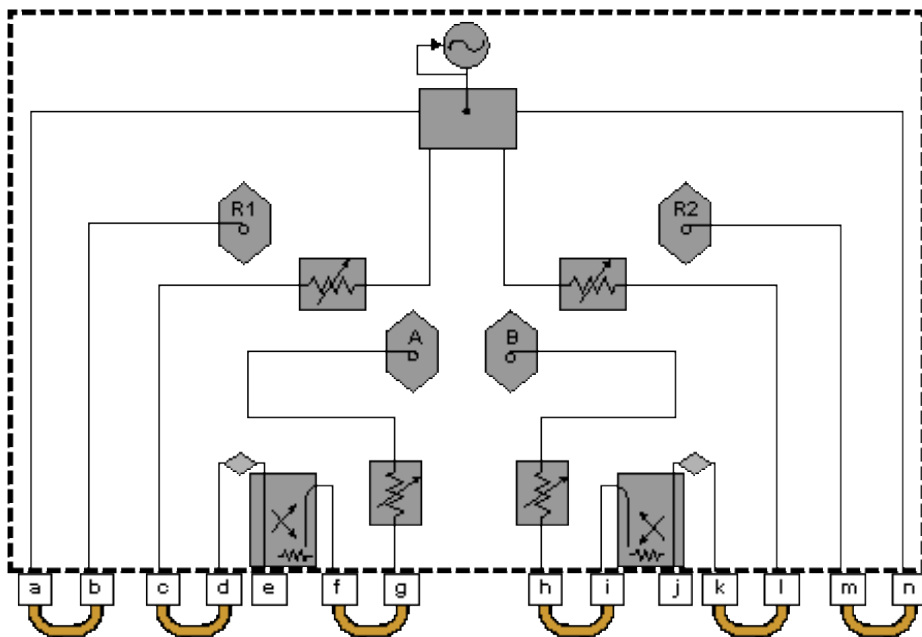

| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

E8361A - Option 014 Configurable Test Set, and Option UNL Extended Power Range and Bias - Tees, and Option 016 Receiver Attenuators, and Option 081 Reference Channel Transfer Switch

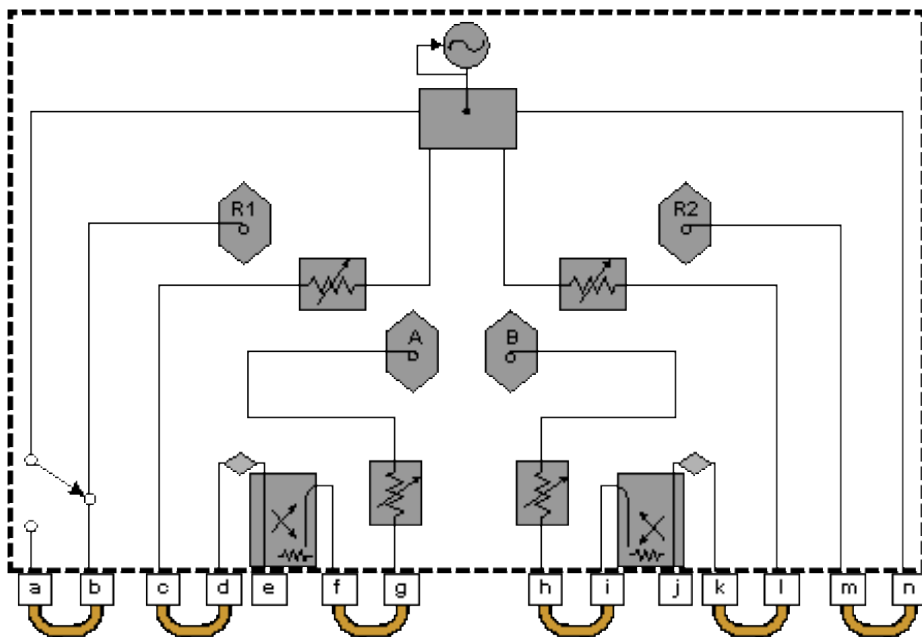

| <b>Item</b> | <b>Description</b> | <b>Item</b> | <b>Description</b> |
|-------------|--------------------|-------------|--------------------|
| <b>a</b>    | SOURCE OUT         | <b>h</b>    | RCVR B IN          |
| <b>b</b>    | RCVR R1 IN         | <b>i</b>    | CPLR ARM           |
| <b>c</b>    | SOURCE OUT         | <b>j</b>    | PORT 2             |
| <b>d</b>    | CPLR THRU          | <b>k</b>    | CPLR THRU          |
| <b>e</b>    | PORT 1             | <b>l</b>    | SOURCE OUT         |
| <b>f</b>    | CPLR ARM           | <b>m</b>    | RCVR R2 IN         |
| <b>g</b>    | RCVR A IN          | <b>n</b>    | SOURCE OUT         |

# Technical Specifications for the E8362A, E8363A, E8364A

---

Because the E8362A, E8363A, and E8364A network analyzer is no longer produced, the technical specifications are stored only on the Internet. To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "E836xA Specifications"

The uncertainty curves contained in this document apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the [equations](#) used to generate the uncertainty curves.

# Technical Specifications for the E8362B, E8363B, E8364B

(Rev. 2004-08-02)

---

This is a complete list of the E8362B, E8363B, and E8364B network analyzer technical specifications.

- To optimize viewing of uncertainty curves, click the Maximize button.
  - To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "E836xB Specifications"
  - The uncertainty curves contained in this document apply only to the setup conditions listed. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your PNA setup. View the [equations](#) used to generate the uncertainty curves.
- 

## Definitions

### Corrected System Performance

[System Dynamic Range](#)

[Receiver Dynamic Range](#)

[24mm Connectors](#)

[292mm Connectors](#)

[35mm Connectors](#)

[7mm Connectors](#)

[Type-N Connectors](#)

[WR-28 Connectors](#)

[WR-42 Connectors](#)

[WR-62 Connectors](#)

[WR-90 Connectors](#)



### Uncorrected System Performance

[Test Port Output](#)

[Test Port Input](#)

[Dynamic Accuracy](#)

[Group Delay](#)

[General Information](#)

[Measurement Throughput Summary](#)

## [Front-panel Jumper Specs \(Option 014 only\)](#)

## [Test Set Block Diagrams](#)

## [Test Set with Option 014 Block Diagrams](#)

[See Specs for other PNA models](#)

## Definitions

All specifications and characteristics apply over a 25 °C  $\pm$ 5 °C range (unless otherwise stated) and 90 minutes after the instrument has been turned on.

**Specification (spec.):** Warranted performance. Specifications include guardbands to account for the expected statistical performance distribution, measurement uncertainties, and changes in performance due to environmental conditions.

**Characteristic (char.):** A performance parameter that the product is expected to meet before it leaves the factory, but that is not verified in the field and is not covered by the product warranty. A characteristic includes the same guardbands as a specification.

**Typical (typ.):** Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Nominal (nom.):** A general, descriptive term that does not imply a level of performance. It is not covered by the product warranty.

**Calibration:** The process of measuring known standards to characterize a network analyzer's systematic (repeatable) errors.

**Corrected (residual):** Indicates performance after [error correction](#) (calibration). It is determined by the quality of calibration standards and how well "known" they are, plus system repeatability, stability, and noise.

**Uncorrected (raw):** Indicates instrument performance without error correction. The uncorrected performance affects the stability of a [calibration](#).

**Standard:** When referring to the analyzer, this includes no options unless noted otherwise.

---

## Corrected System Performance

The specifications in this section apply for measurements made with the E836xB analyzer with the following conditions:

- 10 Hz IF bandwidth
- No averaging applied to data
- Isolation calibration with an averaging factor of 8

## [System Dynamic Range](#)

## [Receiver Dynamic Range](#)

## [24mm Connectors](#)

## [292mm Connectors](#)

## [35mm Connectors](#)

## [7mm-Connectors](#)

**Type-N Connectors**

**WR-28 Connectors**

**WR-42-Connectors**

**WR-62 Connectors**

**WR-90 Connectors**

**Table 1. System Dynamic Range<sup>a</sup>**

| Description                                                                 | Specification (dB) at Test Port <sup>b</sup> | Typical (dB) at Direct Receiver Access Input <sup>c</sup> | Supplemental Information                 |
|-----------------------------------------------------------------------------|----------------------------------------------|-----------------------------------------------------------|------------------------------------------|
| <b>Dynamic Range (in a 10 Hz BW)</b>                                        |                                              |                                                           |                                          |
| <b>Standard Configuration and Standard Power Range (E836xB - Standard)</b>  |                                              |                                                           |                                          |
| 10 MHz to 45 MHz <sup>d</sup>                                               | 79                                           | NA                                                        |                                          |
| 45 MHz to 500 MHz <sup>e</sup>                                              | 94                                           | NA                                                        |                                          |
| 500 MHz to 2 GHz                                                            | 119                                          | NA                                                        |                                          |
| 2 GHz to 10 GHz                                                             | 122                                          | NA                                                        |                                          |
| 10 GHz to 20 GHz                                                            | 123                                          | NA                                                        |                                          |
| 20 GHz to 30 GHz                                                            | 114                                          | NA                                                        |                                          |
| 30 GHz to 40 GHz                                                            | 110                                          | NA                                                        |                                          |
| 40 GHz to 45 GHz                                                            | 109                                          | NA                                                        |                                          |
| 45 GHz to 50 GHz                                                            | 104                                          | NA                                                        |                                          |
| <b>Configurable Test Set and Standard Power Range (E836xB - Option 014)</b> |                                              |                                                           |                                          |
| 10 MHz to 45 MHz <sup>d</sup>                                               | 79                                           | 129                                                       | Option 016 degrades performance by 2 dB. |
| 45 MHz to 500 MHz <sup>e</sup>                                              | 94                                           | 132                                                       |                                          |
| 500 MHz to 2 GHz                                                            | 119                                          | 138                                                       |                                          |
| 2 GHz to 10 GHz                                                             | 122                                          | 137                                                       |                                          |
| 10 GHz to 20 GHz                                                            | 121                                          | 136                                                       |                                          |
| 20 GHz to 30 GHz                                                            | 111                                          | 123                                                       |                                          |
| 30 GHz to 40 GHz                                                            | 107                                          | 119                                                       |                                          |
| 40 GHz to 45 GHz                                                            | 105                                          | 116                                                       |                                          |
| 45 GHz to 50 GHz                                                            | 100                                          | 111                                                       |                                          |

### Standard Configuration and Extended Power Range & Bias-Tees

#### (E836xB - Option UNL)

|                                |     |    |                                          |
|--------------------------------|-----|----|------------------------------------------|
| 10 MHz to 45 MHz <sup>d</sup>  | 79  | NA | Option 016 degrades performance by 2 dB. |
| 45 MHz to 500 MHz <sup>e</sup> | 92  | NA |                                          |
| 500 MHz to 2 GHz               | 117 | NA |                                          |
| 2 GHz to 10 GHz                | 120 | NA |                                          |
| 10 GHz to 20 GHz               | 121 | NA |                                          |
| 20 GHz to 30 GHz               | 112 | NA |                                          |
| 30 GHz to 40 GHz               | 108 | NA |                                          |
| 40 GHz to 45 GHz               | 105 | NA |                                          |
| 45 GHz to 50 GHz               | 99  | NA |                                          |

### Configurable Test Set and Extended Power Range & Bias-Tees

#### (E836xB - Option 014/UNL)

|                                   |     |     |                                          |
|-----------------------------------|-----|-----|------------------------------------------|
| 10 MHz to 45 MHz <sup>d</sup>     | 79  | 129 | Option 016 degrades performance by 2 dB. |
| 45 MHz to 500 MHz <sup>e, f</sup> | 92  | 130 |                                          |
| 500 MHz to 2 GHz <sup>f</sup>     | 117 | 136 |                                          |
| 2 GHz to 10 GHz <sup>f</sup>      | 120 | 135 |                                          |
| 10 GHz to 20 GHz <sup>g</sup>     | 119 | 134 |                                          |
| 20 GHz to 30 GHz                  | 109 | 121 |                                          |
| 30 GHz to 40 GHz                  | 105 | 117 |                                          |
| 40 GHz to 45 GHz                  | 101 | 112 |                                          |
| 45 GHz to 50 GHz                  | 95  | 106 |                                          |

a The system dynamic range is calculated as the difference between the noise floor and the source maximum output power. System dynamic range is a specification when the source is set to Port 1, and a characteristic when the source is set to Port 2. The effective dynamic range must take measurement uncertainties and interfering signals into account as well as the insertion loss resulting from a thru cable connected between Port 1 and Port 2..

b The test port system dynamic range is calculated as the difference between the test port noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account as well as the insertion loss resulting from a thru cable connected between Port 1 and Port 2..

c The direct receiver access input system dynamic range is calculated as the difference between the receiver access input noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its damage level. When the analyzer is in segment sweep mode, the analyzer can have predefined frequency segments which will output a higher power level when the extended dynamic range is required (i.e. devices with high insertion loss), and reduced power when receiver damage may occur (i.e. devices with low insertion loss). The extended range is only available in one-path transmission measurements.

d Typical performance.

e May be limited to 100 dB at particular frequencies below 500 MHz due to spurious receiver residuals. Methods are available to regain the full dynamic range.

f E8362B only: Option H11 decreases value by 1 dB.

g E8362B only: Option H11 decreases value by 2 dB.

**Table 2. Receiver Dynamic Range<sup>a</sup>**



| Description                                                                                     | Specification (dB) at Test Port <sup>b</sup> | Typical (dB) at Direct Receiver Access Input <sup>c</sup> |                                          |
|-------------------------------------------------------------------------------------------------|----------------------------------------------|-----------------------------------------------------------|------------------------------------------|
| <b>Dynamic Range (in a 10 Hz BW)</b>                                                            |                                              |                                                           |                                          |
| <b>Standard Configuration and Standard Power Range (E836xB - Standard)</b>                      |                                              |                                                           |                                          |
| <b>OR</b>                                                                                       |                                              |                                                           |                                          |
| <b>Standard Configuration and Extended Power Range &amp; Bias Tees (E836xB - Option UNL)</b>    |                                              |                                                           |                                          |
| 10 MHz to 45 MHz <sup>d</sup>                                                                   | 82                                           | NA                                                        |                                          |
| 45 MHz to 500 MHz <sup>e</sup>                                                                  | 94                                           | NA                                                        |                                          |
| 500 MHz to 2 GHz                                                                                | 119                                          | NA                                                        |                                          |
| 2 GHz to 10 GHz                                                                                 | 122                                          | NA                                                        |                                          |
| 10 GHz to 20 GHz                                                                                | 125                                          | NA                                                        |                                          |
| 20 GHz to 30 GHz                                                                                | 114                                          | NA                                                        | Option 016 degrades performance by 2 dB. |
| 30 GHz to 40 GHz                                                                                | 111                                          | NA                                                        |                                          |
| 40 GHz to 50 GHz                                                                                | 111                                          | NA                                                        |                                          |
| <b>Configurable Test Set and Standard Power Range (E836xB - Option 014)</b>                     |                                              |                                                           |                                          |
| <b>OR</b>                                                                                       |                                              |                                                           |                                          |
| <b>Configurable Test Set and Extended Power Range &amp; Bias Tees (E836xB - Option 014/UNL)</b> |                                              |                                                           |                                          |
| 10 MHz to 45 MHz <sup>d</sup>                                                                   | 82                                           | 132                                                       |                                          |
| 45 MHz to 500 MHz <sup>e</sup>                                                                  | 94                                           | 132                                                       |                                          |
| 500 MHz to 2 GHz                                                                                | 119                                          | 138                                                       |                                          |
| 2 GHz to 10 GHz                                                                                 | 122                                          | 137                                                       |                                          |
| 10 GHz to 20 GHz                                                                                | 124                                          | 139                                                       |                                          |
| 20 GHz to 30 GHz                                                                                | 113                                          | 125                                                       | Option 016 degrades performance by 2 dB. |
| 30 GHz to 40 GHz                                                                                | 110                                          | 122                                                       |                                          |
| 40 GHz to 50 GHz                                                                                | 109                                          | 120                                                       |                                          |

a The receiver dynamic range is calculated as the difference between the noise floor and the receiver maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account.

b The test port receiver dynamic range is calculated as the difference between the test port noise floor and the receiver maximum input level. The effective dynamic range must take measurement uncertainties and interfering signals into account.

c The direct receiver access input receiver dynamic range is calculated as the difference between the direct receiver access input noise floor and the receiver maximum input level. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its compression or damage level. When the analyzer is in segment sweep mode, the analyzer can have predefined frequency segments which will output a higher power level when the extended dynamic range is required (i.e. devices with high insertion loss), and reduced power when compression or receiver damage may occur (i.e. devices with low insertion loss). The extended range is only available in one-path transmission measurements.

d Typical performance.

e May be degraded by 10 dB at particular frequencies (multiples of 5 MHz) below 500 MHz due to spurious receiver residuals. Methods are available to regain the full dynamic range.

**Note:** This E836xB document provides technical specifications for the following calibration kits only: 85056A,

85056D, 85056K, 85052B, 85052C, 85052D, 85050B, 85050C, 85050D, 85054B, 85054D, K11644A, P11644A, R11644A, and the X11644A.

**Table 33. Uncorrected System Performance<sup>a</sup>**

Specifications apply over environmental temperature of 23° ±3 °C, with < 1 °C deviation from the calibration temperature

| Description                                   | Specification | Supplemental Information |
|-----------------------------------------------|---------------|--------------------------|
| <b>Directivity</b>                            |               |                          |
| 10 MHz to 45 MHz <sup>b</sup>                 | 23 dB         |                          |
| 45 MHz to 2 GHz                               | 24 dB         |                          |
| 2 GHz to 10 GHz                               | 22 dB         |                          |
| 10 GHz to 20 GHz                              | 16 dB         |                          |
| 20 GHz to 40 GHz                              | 16 dB         |                          |
| 40 GHz to 45 GHz                              | 15 dB         |                          |
| 45 GHz to 50 GHz                              | 13 dB         |                          |
| <b>Source Match - Standard</b>                |               |                          |
| 10 MHz to 45 MHz <sup>b</sup>                 | 11 dB         |                          |
| 45 MHz to 2 GHz                               | 23 dB         |                          |
| 2 GHz to 10 GHz                               | 16 dB         |                          |
| 10 GHz to 20 GHz                              | 14 dB         |                          |
| 20 GHz to 40 GHz                              | 10 dB         |                          |
| 40 GHz to 45 GHz                              | 9 dB          |                          |
| 45 GHz to 50 GHz                              | 7.5 dB        |                          |
| <b>Source Match - Opt UNL, 014 or 014/UNL</b> |               |                          |
| 10 MHz to 45 MHz <sup>b</sup>                 | 11 dB         |                          |
| 45 MHz to 2 GHz                               | 18 dB         |                          |
| 2 GHz to 10 GHz                               | 14 dB         |                          |
| 10 GHz to 20 GHz                              | 12 dB         |                          |
| 20 GHz to 40 GHz                              | 9 dB          |                          |
| 40 GHz to 45 GHz                              | 8 dB          |                          |

|                                             |       |                 |
|---------------------------------------------|-------|-----------------|
| 45 GHz to 50 GHz                            | 6 dB  |                 |
| <b>Load Match - Standard</b>                |       |                 |
| 10 MHz to 45 MHz <sup>b</sup>               | 11 dB |                 |
| 45 MHz to 2 GHz                             | 23 dB |                 |
| 2 GHz to 10 GHz                             | 14 dB |                 |
| 10 GHz to 20 GHz                            | 10 dB |                 |
| 20 GHz to 40 GHz                            | 9 dB  |                 |
| 40 GHz to 45 GHz                            | 9 dB  |                 |
| 45 GHz to 50 GHz                            | 8 dB  |                 |
| <b>Load Match - Opt UNL, 014 or 014/UNL</b> |       |                 |
| 10 MHz to 45 MHz <sup>b</sup>               | 11 dB |                 |
| 45 MHz to 2 GHz                             | 17 dB |                 |
| 2 GHz to 10 GHz                             | 13 dB |                 |
| 10 GHz to 20 GHz                            | 10 dB |                 |
| 20 GHz to 40 GHz                            | 9 dB  |                 |
| 40 GHz to 45 GHz                            | 9 dB  |                 |
| 45 GHz to 50 GHz                            | 7 dB  |                 |
| <b>Reflection Tracking</b>                  |       |                 |
|                                             |       | <b>Typical:</b> |
| 10 MHz to 45 MHz                            |       | ±1.5 dB         |
| 45 MHz to 20 GHz                            |       | ±1.5 dB         |
| 20 GHz to 40 GHz                            |       | ±1.5 dB         |
| 40 GHz to 50 GHz                            |       | ±2.0 dB         |
| <b>Transmission Tracking<sup>c</sup></b>    |       |                 |
|                                             |       | <b>Typical:</b> |
| 10 MHz to 45 MHz                            |       | ±3.0 dB         |
| 45 MHz to 2 GHz                             |       | ±1.5 dB         |

|                                                  |         |         |
|--------------------------------------------------|---------|---------|
| 2 GHz to 10 GHz                                  |         | ±2.0 dB |
| 10 GHz to 20 GHz                                 |         | ±2.5 dB |
| 20 GHz to 40 GHz                                 |         | ±3.5 dB |
| 40 GHz to 45 GHz                                 |         | ±4.0 dB |
| 45 GHz to 50 GHz                                 |         | ±4.5 dB |
| <b>Crosstalk<sup>d</sup> - Standard</b>          |         |         |
| 10 MHz to 45 MHz <sup>b</sup>                    | -65 dB  |         |
| 45 MHz to 1 GHz                                  | -85 dB  |         |
| 1 GHz to 2 GHz                                   | -100 dB |         |
| 2 GHz to 20 GHz                                  | -110 dB |         |
| 20 GHz to 40 GHz                                 | -108 dB |         |
| 40 GHz to 45 GHz                                 | -105 dB |         |
| 45 GHz to 50 GHz                                 | -100 dB |         |
| <b>Crosstalk<sup>d</sup> - Option UNL or 014</b> |         |         |
| 10 MHz to 45 MHz <sup>b</sup>                    | -65 dB  |         |
| 45 MHz to 1 GHz                                  | -85 dB  |         |
| 1 GHz to 2 GHz                                   | -100 dB |         |
| 2 GHz to 20 GHz                                  | -109 dB |         |
| 20 GHz to 40 GHz                                 | -106 dB |         |
| 40 GHz to 45 GHz                                 | -103 dB |         |
| 45 GHz to 50 GHz                                 | -98 dB  |         |
| <b>Crosstalk<sup>d</sup> - Option 014/UNL</b>    |         |         |
| 10 MHz to 45 MHz <sup>b</sup>                    | -65 dB  |         |
| 45 MHz to 1 GHz                                  | -85 dB  |         |
| 1 GHz to 2 GHz                                   | -98 dB  |         |
| 2 GHz to 10 GHz                                  | -108 dB |         |
| 10 GHz to 20 GHz                                 | -107 dB |         |

|                                                     |         |                 |
|-----------------------------------------------------|---------|-----------------|
| 20 GHz to 40 GHz                                    | -104 dB |                 |
| 40 GHz to 45 GHz                                    | -100 dB |                 |
| 45 GHz to 50 GHz                                    | -95 dB  |                 |
| <b>Crosstalk - Option 080 enabled<sup>b,e</sup></b> |         |                 |
|                                                     |         | <b>Typical:</b> |
| 10 MHz to 45 MHz                                    |         | -65             |
| 45 MHz to 1 GHz                                     |         | -85             |
| 1 GHz to 2 GHz                                      |         | -100            |
| 2 GHz to 10 GHz                                     |         | -109            |
| 10 GHz to 20 GHz                                    |         | -110            |
| 20 GHz to 40 GHz                                    |         | -106            |
| 40 GHz to 45 GHz                                    |         | -103            |
| 45 GHz to 50 GHz                                    |         | -98             |

a Specifications apply over environment temperature of 23°C +/- 3°C, with less than 1°C deviation from the calibration temperature.

b Typical performance.

c Transmission tracking performance is strongly dependent on cable used. These typical specifications are based on the use of the Agilent thru cable (part number 85133-60016).

d Measurement conditions: normalized to a thru, measured with two shorts, 10 Hz IF bandwidth, averaging factor of 16, alternate mode, source power set to the lesser of the maximum power out or the maximum receiver power.

e 0 Hz offset.

**Table 34. Test Port Output**

| Description                      | Specification    |         |         |             | Supplemental |
|----------------------------------|------------------|---------|---------|-------------|--------------|
|                                  | Standard         | Opt 014 | Opt UNL | Opt 014/UNL |              |
| <b>Frequency Range</b>           |                  |         |         |             |              |
|                                  |                  |         |         |             |              |
| E8362B                           | 10 MHz to 20 GHz |         |         |             |              |
| E8363B                           | 10 MHz to 40 GHz |         |         |             |              |
| E8364B                           | 10 MHz to 50 GHz |         |         |             |              |
| <b>Nominal Power<sup>c</sup></b> |                  |         |         |             |              |
| E8362B                           | 0 dBm            | -5 dBm  | -5 dBm  | -5 dBm      |              |

|                                          |         |         |         |         |                                                                   |
|------------------------------------------|---------|---------|---------|---------|-------------------------------------------------------------------|
| E8363/4B                                 | -12 dBm | -17 dBm | -17 dBm | -17 dBm |                                                                   |
| <b>Frequency Resolution</b>              |         |         |         |         |                                                                   |
|                                          | 1 Hz    |         |         |         |                                                                   |
| <b>CW Accuracy</b>                       |         |         |         |         |                                                                   |
|                                          | ±1 ppm  |         |         |         |                                                                   |
| <b>Frequency Stability</b>               |         |         |         |         |                                                                   |
|                                          |         |         |         |         | ±0.05 ppm. - 10° to 70° C, typical; ±0.1 ppm/yr maximum, typical  |
| <b>Power Level Accuracy<sup>a</sup></b>  |         |         |         |         |                                                                   |
| 10 MHz to 45 MHz <sup>b</sup>            | ±2.0 dB | ±2.0 dB | ±2.0 dB | ±2.0 dB |                                                                   |
| 45 MHz to 10 GHz                         | ±1.5 dB | ±1.5 dB | ±1.5 dB | ±1.5 dB | Variation from nominal power in range 0 (step attenuator at 0 dB) |
| 10 GHz to 20 GHz                         | ±2.0 dB | ±2.0 dB | ±2.0 dB | ±2.0 dB |                                                                   |
| 20 GHz to 40 GHz                         | ±3.0 dB | ±3.0 dB | ±3.0 dB | ±3.0 dB |                                                                   |
| 40 GHz to 45 GHz                         | ±3.0 dB | ±3.5 dB | ±3.0 dB | ±3.5 dB |                                                                   |
| 45 GHz to 50 GHz                         | ±3.0 dB | ±4.0 dB | ±3.0 dB | ±4.0 dB |                                                                   |
| <b>Power Level Linearity<sup>d</sup></b> |         |         |         |         |                                                                   |

|                                      |                        |                |                |                            |                                                                        |
|--------------------------------------|------------------------|----------------|----------------|----------------------------|------------------------------------------------------------------------|
| 10 MHz to 45 MHz <sup>b</sup>        | +/-1.0 dB <sup>g</sup> |                |                |                            | Test reference is at the nominal power level (step attenuator at 0 dB) |
| 45 MHz to 20 GHz                     | +/-1.0 dB <sup>g</sup> |                |                |                            |                                                                        |
| 20 GHz to 40 GHz                     | +/-1.0 dB <sup>g</sup> |                |                |                            |                                                                        |
| 40 GHz to 50 GHz                     | +/-1.0 dB <sup>g</sup> |                |                |                            |                                                                        |
| <b>Power Range<sup>a, e, f</sup></b> |                        |                |                |                            |                                                                        |
| 10 MHz to 45 MHz <sup>b</sup>        | -25 to +2 dBm          | -25 to +2 dBm  | -87 to +2 dBm  | -87 to +2 dBm              |                                                                        |
| 45 MHz to 10 GHz                     | -25 to +5 dBm          | -25 to +5 dBm  | -87 to +3 dBm  | -87 to +3 dBm <sup>h</sup> |                                                                        |
| 10 GHz to 20 GHz                     | -24 to +3 dBm          | -25 to +2 dBm  | -86 to +1 dBm  | -87 to 0 dBm <sup>i</sup>  |                                                                        |
| 20 GHz to 30 GHz                     | -23 to 0 dBm           | -25 to -2 dBm  | -85 to -2 dBm  | -87 to -4 dBm              |                                                                        |
| 30 GHz to 40 GHz                     | -23 to -4 dBm          | -25 to -6 dBm  | -85 to -6 dBm  | -87 to -8 dBm              |                                                                        |
| 40 GHz to 45 GHz                     | -25 to -5 dBm          | -27 to -7 dBm  | -87 to -9 dBm  | -87 to -11 dBm             |                                                                        |
| 45 GHz to 50 GHz                     | -25 to -10 dBm         | -27 to -12 dBm | -87 to -15 dBm | -87 to -17 dBm             |                                                                        |
| <b>Power Sweep Range (ALC)</b>       |                        |                |                |                            |                                                                        |
| 10 MHz to 45 MHz <sup>b</sup>        | 27 dB                  | 27 dB          | 29 dB          | 29 dB                      |                                                                        |

|                                                                                            |         |       |       |                    |                                                                                                       |
|--------------------------------------------------------------------------------------------|---------|-------|-------|--------------------|-------------------------------------------------------------------------------------------------------|
| 45 MHz to 10 GHz                                                                           | 30 dB   | 30 dB | 30 dB | 30 dB <sup>j</sup> | ALC range starts at maximum leveled output power and decreases by power level indicated in the table. |
| 10 GHz to 20 GHz                                                                           | 27 dB   | 27 dB | 27 dB | 27 dB <sup>k</sup> |                                                                                                       |
| 20 GHz to 30 GHz                                                                           | 23 dB   | 23 dB | 23 dB | 23 dB              |                                                                                                       |
| 30 GHz to 40 GHz                                                                           | 19 dB   | 19 dB | 19 dB | 19 dB              |                                                                                                       |
| 40 GHz to 45 GHz                                                                           | 20 dB   | 20 dB | 18 dB | 16 dB              |                                                                                                       |
| 45 GHz to 50 GHz                                                                           | 15 dB   | 15 dB | 12 dB | 10 dB              |                                                                                                       |
| <b>Power Resolution</b>                                                                    |         |       |       |                    |                                                                                                       |
|                                                                                            | 0.01 dB |       |       |                    |                                                                                                       |
| <b>Phase Noise</b>                                                                         |         |       |       |                    |                                                                                                       |
| <b>1 kHz offset from center frequency, nominal power at test port</b>                      |         |       |       |                    |                                                                                                       |
|                                                                                            |         |       |       |                    | <b>Typical:</b>                                                                                       |
| 10 MHz to 10 GHz                                                                           |         |       |       |                    | -60 dBc                                                                                               |
| 10 GHz to 20 GHz                                                                           |         |       |       |                    | -55 dBc                                                                                               |
| 20 GHz to 50 GHz                                                                           |         |       |       |                    | -50 dBc                                                                                               |
| <b>1 kHz offset from center frequency, nominal power at test port - Option 080 enabled</b> |         |       |       |                    |                                                                                                       |
|                                                                                            |         |       |       |                    | <b>Typical:</b>                                                                                       |
| 10 MHz to 10 GHz                                                                           |         |       |       |                    | -60 dBc                                                                                               |
| 10 GHz to 20 GHz                                                                           |         |       |       |                    | -60 dBc                                                                                               |
| 20 GHz to 50 GHz                                                                           |         |       |       |                    | -50 dBc                                                                                               |
| <b>10 kHz offset from center frequency, nominal power at test port</b>                     |         |       |       |                    |                                                                                                       |
|                                                                                            |         |       |       |                    | <b>Typical:</b>                                                                                       |
| 10 MHz to 45 MHz                                                                           |         |       |       |                    | -70 dBc                                                                                               |
| 45 MHz to 10 GHz                                                                           |         |       |       |                    | -70 dBc                                                                                               |
| 10 GHz to 20 GHz                                                                           |         |       |       |                    | -65 dBc                                                                                               |



|                                                                                              |  |  |  |  |                 |
|----------------------------------------------------------------------------------------------|--|--|--|--|-----------------|
| 20 GHz to 40 GHz                                                                             |  |  |  |  | -55 dBc         |
| 40 GHz to 50 GHz                                                                             |  |  |  |  | -55 dBc         |
| <b>10 kHz offset from center frequency, nominal power at test port - Option 080 enabled</b>  |  |  |  |  |                 |
|                                                                                              |  |  |  |  | <b>Typical:</b> |
| 10 MHz to 45 MHz                                                                             |  |  |  |  | -70 dBc         |
| 45 MHz to 10 GHz                                                                             |  |  |  |  | -70 dBc         |
| 10 GHz to 20 GHz                                                                             |  |  |  |  | -65 dBc         |
| 20 GHz to 40 GHz                                                                             |  |  |  |  | -55 dBc         |
| 40 GHz to 50 GHz                                                                             |  |  |  |  | -55 dBc         |
| <b>100 kHz offset from center frequency, nominal power at test port</b>                      |  |  |  |  |                 |
|                                                                                              |  |  |  |  | <b>Typical:</b> |
| 10 MHz to 10 GHz                                                                             |  |  |  |  | -60 dBc         |
| 10 GHz to 20 GHz                                                                             |  |  |  |  | -55 dBc         |
| 20 GHz to 50 GHz                                                                             |  |  |  |  | -50 dBc         |
| <b>100 kHz offset from center frequency, nominal power at test port - Option 080 enabled</b> |  |  |  |  |                 |
|                                                                                              |  |  |  |  | <b>Typical:</b> |
| 10 MHz to 10 GHz                                                                             |  |  |  |  | -75 dBc         |
| 10 GHz to 20 GHz                                                                             |  |  |  |  | -70 dBc         |
| 20 GHz to 50 GHz                                                                             |  |  |  |  | -65 dBc         |
| <b>1 MHz offset from center frequency, nominal power at test port</b>                        |  |  |  |  |                 |
|                                                                                              |  |  |  |  | <b>Typical:</b> |
| 10 MHz to 10 GHz                                                                             |  |  |  |  | -106 dBc        |
| 10 GHz to 20 GHz                                                                             |  |  |  |  | -103 dBc        |
| 20 GHz to 50 GHz                                                                             |  |  |  |  | -90 dBc         |
| <b>1 MHz offset from center frequency, nominal power at test port - Option 080 enabled</b>   |  |  |  |  |                 |
|                                                                                              |  |  |  |  | <b>Typical:</b> |
| 10 MHz to 10 GHz                                                                             |  |  |  |  | -103 dBc        |

|                                                        |  |  |  |  |                                                           |
|--------------------------------------------------------|--|--|--|--|-----------------------------------------------------------|
| 10 GHz to 20 GHz                                       |  |  |  |  | -97 dBc                                                   |
| 20 GHz to 50 GHz                                       |  |  |  |  | -85 dBc                                                   |
| <b>Harmonics (2nd or 3rd)</b>                          |  |  |  |  |                                                           |
|                                                        |  |  |  |  | -23 dBc<br>typical, in<br>power range 0                   |
| <b>Non-Harmonic Spurious (at Nominal Output Power)</b> |  |  |  |  |                                                           |
| 10 MHz to 45 MHz                                       |  |  |  |  | -50 dBc<br>typical, for<br>offset<br>frequency > 1<br>kHz |
| 45 MHz to 20 GHz                                       |  |  |  |  | -50 dBc<br>typical, for<br>offset<br>frequency > 1<br>kHz |
| 20 GHz to 40 GHz                                       |  |  |  |  | -30 dBc<br>typical, for<br>offset<br>frequency > 1<br>kHz |
| 40 GHz to 50 GHz                                       |  |  |  |  | -30 dBc<br>typical, for<br>offset<br>frequency > 1<br>kHz |

a Test port output is a specification when the source is set to Port 1, and a characteristic when the source is set to Port 2.

b Typical performance.

c Preset power.

d Power Level Linearity is a specification when the source is set to Port 1, and a typical when the source is set to Port 2.

e Test port power is specified into nominal 50 ohms.

f Power to which the source can be set and phase lock is assured.

g +/-1.5 dB for power <= -23 dBm.

h E8362B only: Option H11 decreases maximum power level by 1 dB.

i E8362B only: Option H11 decreases maximum power level by 2 dB.

j E8362B only: Option H11 decreases power level by 1 dB.

k E8362B only: Option H11 decreases power level by 2 dB.

**Table 35: Test Port Input**

| Description | Specification |         |         |             | Supplemental |
|-------------|---------------|---------|---------|-------------|--------------|
|             | Standard      | Opt 014 | Opt UNL | Opt 014/UNL |              |
|             |               |         |         |             |              |

| <b>Test Port Noise Floor<sup>a</sup></b> |           |           |           |           |                                          |
|------------------------------------------|-----------|-----------|-----------|-----------|------------------------------------------|
| <b>10 Hz IF Bandwidth</b>                |           |           |           |           |                                          |
| 10 MHz to 45 MHz <sup>b</sup>            | <-77 dBm  | <-77 dBm  | <-77 dBm  | <-77 dBm  |                                          |
| 45 MHz to 500 MHz <sup>c</sup>           | <-89 dBm  | <-89 dBm  | <-89 dBm  | <-89 dBm  |                                          |
| 500 MHz to 2 GHz                         | <-114 dBm | <-114 dBm | <-114 dBm | <-114 dBm |                                          |
| 2 GHz to 10 GHz                          | <-117 dBm | <-117 dBm | <-117 dBm | <-117 dBm |                                          |
| 10 GHz to 20 GHz                         | <-120 dBm | <-119 dBm | <-120 dBm | <-119 dBm |                                          |
| 20 GHz to 40 GHz                         | <-114 dBm | <-113 dBm | <-114 dBm | <-113 dBm | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz                         | <-114 dBm | <-112 dBm | <-114 dBm | <-112 dBm |                                          |
| <b>1 KHz IF Bandwidth</b>                |           |           |           |           |                                          |
| 10 MHz to 45 MHz <sup>b</sup>            | <-57 dBm  | <-57 dBm  | <-57 dBm  | <-57 dBm  |                                          |
| 45 MHz to 500 MHz <sup>c</sup>           | <-69 dBm  | <-69 dBm  | <-69 dBm  | <-69 dBm  |                                          |
| 500 MHz to 2 GHz                         | <-94 dBm  | <-94 dBm  | <-94 dBm  | <-94 dBm  |                                          |
| 2 GHz to 10 GHz                          | <-97 dBm  | <-97 dBm  | <-97 dBm  | <-97 dBm  |                                          |
| 10 GHz to 20 GHz                         | <-100 dBm | <-99 dBm  | <-100 dBm | <-99 dBm  |                                          |
| 20 GHz to 40 GHz                         | <-94 dBm  | <-93 dBm  | <-94 dBm  | <-93 dBm  | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz                         | <-94 dBm  | <-92 dBm  | <-94 dBm  | <-92 dBm  |                                          |

**Test Port Noise Floor<sup>a,b</sup> Option 080 enabled<sup>d</sup>**

**10 Hz IF Bandwidth**

|                                |           |           |           |           |                                          |
|--------------------------------|-----------|-----------|-----------|-----------|------------------------------------------|
| 10 MHz to 45 MHz <sup>b</sup>  | <-77 dBm  | <-77 dBm  | <-77 dBm  | <-77 dBm  |                                          |
| 45 MHz to 500 MHz <sup>c</sup> | <-88 dBm  | <-88 dBm  | <-88 dBm  | <-88 dBm  |                                          |
| 500 MHz to 2 GHz               | <-113 dBm | <-113 dBm | <-113 dBm | <-113 dBm |                                          |
| 2 GHz to 10 GHz                | <-116 dBm | <-116 dBm | <-116 dBm | <-116 dBm |                                          |
| 10 GHz to 20 GHz               | <-118 dBm | <-118 dBm | <-118 dBm | <-118 dBm |                                          |
| 20 GHz to 40 GHz               | <-112 dBm | <-112 dBm | <-112 dBm | <-112 dBm | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz               | <-111 dBm | <-111 dBm | <-111 dBm | <-111 dBm |                                          |

**1 KHz IF Bandwidth**

|                                |          |          |          |          |                                          |
|--------------------------------|----------|----------|----------|----------|------------------------------------------|
| 10 MHz to 45 MHz <sup>b</sup>  | <-57 dBm | <-57 dBm | <-57 dBm | <-57 dBm |                                          |
| 45 MHz to 500 MHz <sup>c</sup> | <-68 dBm | <-68 dBm | <-68 dBm | <-68 dBm |                                          |
| 500 MHz to 2 GHz               | <-93 dBm | <-93 dBm | <-93 dBm | <-93 dBm |                                          |
| 2 GHz to 10 GHz                | <-96 dBm | <-96 dBm | <-96 dBm | <-96 dBm |                                          |
| 10 GHz to 20 GHz               | <-98 dBm | <-98 dBm | <-98 dBm | <-98 dBm |                                          |
| 20 GHz to 40 GHz               | <-92 dBm | <-92 dBm | <-92 dBm | <-92 dBm | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz               | <-91 dBm | <-91 dBm | <-91 dBm | <-91 dBm |                                          |

| Direct Receiver Access Input Noise Floor <sup>a,b</sup>                                   |  |           |  |           |                                          |
|-------------------------------------------------------------------------------------------|--|-----------|--|-----------|------------------------------------------|
| <b>10 Hz IF Bandwidth</b>                                                                 |  |           |  |           |                                          |
| 10 MHz to 45 MHz                                                                          |  | <-127 dBm |  | <-127 dBm |                                          |
| 45 MHz to 500 MHz <sup>c</sup>                                                            |  | <-127 dBm |  | <-127 dBm |                                          |
| 500 MHz to 2 GHz                                                                          |  | <-133 dBm |  | <-133 dBm |                                          |
| 2 GHz to 10 GHz                                                                           |  | <-132 dBm |  | <-132 dBm |                                          |
| 10 GHz to 20 GHz                                                                          |  | <-134 dBm |  | <-134 dBm |                                          |
| 20 GHz to 40 GHz                                                                          |  | <-125 dBm |  | <-125 dBm | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz                                                                          |  | <-123 dBm |  | <-123 dBm |                                          |
| <b>1 KHz IF Bandwidth</b>                                                                 |  |           |  |           |                                          |
| 10 MHz to 45 MHz                                                                          |  | <-107 dBm |  | <-107 dBm |                                          |
| 45 MHz to 500 MHz <sup>c</sup>                                                            |  | <-107 dBm |  | <-107 dBm |                                          |
| 500 MHz to 2 GHz                                                                          |  | <-113 dBm |  | <-113 dBm |                                          |
| 2 GHz to 10 GHz                                                                           |  | <-112 dBm |  | <-112 dBm |                                          |
| 10 GHz to 20 GHz                                                                          |  | <-114 dBm |  | <-114 dBm |                                          |
| 20 GHz to 40 GHz                                                                          |  | <-105 dBm |  | <-105 dBm | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz                                                                          |  | <-103 dBm |  | <-103 dBm |                                          |
| Direct Receiver Access Input Noise Floor <sup>a,b</sup> - Option 080 enabled <sup>d</sup> |  |           |  |           |                                          |

| 10 Hz IF Bandwidth             |                                                       |           |  |           |                                          |
|--------------------------------|-------------------------------------------------------|-----------|--|-----------|------------------------------------------|
| 10 MHz to 45 MHz               |                                                       | <-127 dBm |  | <-127 dBm |                                          |
| 45 MHz to 500 MHz <sup>C</sup> |                                                       | <-126 dBm |  | <-126 dBm |                                          |
| 500 MHz to 2 GHz               |                                                       | <-132 dBm |  | <-132 dBm |                                          |
| 2 GHz to 10 GHz                |                                                       | <-131 dBm |  | <-131 dBm |                                          |
| 10 GHz to 20 GHz               |                                                       | <-133 dBm |  | <-133 dBm |                                          |
| 20 GHz to 40 GHz               |                                                       | <-124 dBm |  | <-124 dBm | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz               |                                                       | <-122 dBm |  | <-122 dBm |                                          |
| 1 KHz IF Bandwidth             |                                                       |           |  |           |                                          |
| 10 MHz to 45 MHz               |                                                       | <-107 dBm |  | <-107 dBm |                                          |
| 45 MHz to 500 MHz <sup>C</sup> |                                                       | <-106 dBm |  | <-106 dBm |                                          |
| 500 MHz to 2 GHz               |                                                       | <-112 dBm |  | <-112 dBm |                                          |
| 2 GHz to 10 GHz                |                                                       | <-111 dBm |  | <-111 dBm |                                          |
| 10 GHz to 20 GHz               |                                                       | <-113 dBm |  | <-113 dBm |                                          |
| 20 GHz to 40 GHz               |                                                       | <-104 dBm |  | <-104 dBm | Option 016 degrades performance by 2 dB. |
| 40 GHz to 50 GHz               |                                                       | <-102 dBm |  | <-102 dBm |                                          |
| Receiver Compression Level     |                                                       |           |  |           |                                          |
| 10 MHz to 20 GHz               | <0.1 dB at -5 dBm <sup>G</sup> and <0.45 dB at +5 dBm |           |  |           |                                          |

|                                                                  |                                                          |                                   |
|------------------------------------------------------------------|----------------------------------------------------------|-----------------------------------|
| 20 GHz to 30 GHz                                                 | <0.1 dB at -9.5 dBm <sup>g</sup> and <0.45 dB at 0 dBm   |                                   |
| 30 GHz to 40 GHz                                                 | <0.1 dB at -12.5 dBm <sup>g</sup> and <0.45 dB at -3 dBm |                                   |
| 40 GHz to 50 GHz                                                 | <0.1 dB at -12.5 dBm <sup>g</sup> and <0.45 dB at -3 dBm |                                   |
| <b>System Compression Level</b>                                  |                                                          |                                   |
|                                                                  | maximum output power                                     | See <u>dynamic accuracy</u> table |
| <b>Third Order Intercept - Tone spacing from 100 kHz - 5 MHz</b> |                                                          |                                   |
|                                                                  |                                                          | <b>Typical</b>                    |
| 10 MHz to 150 MHz                                                |                                                          | +33 dBm                           |
| 150 MHz to 300 MHz                                               |                                                          | +34 dBm                           |
| 300 MHz to 500 MHz                                               |                                                          | +30 dBm                           |
| 500 MHz to 20 GHz                                                |                                                          | +24 dBm                           |
| 20 to 40 GHz                                                     |                                                          | +18 dBm                           |
| 40 to 50 GHz                                                     |                                                          | +15 dBm                           |
| <b>Third Order Intercept - Tone spacing from 5 MHz - 20 MHz</b>  |                                                          |                                   |
|                                                                  |                                                          | <b>Typical</b>                    |
| 10 MHz to 500 MHz                                                |                                                          | +20 dBm                           |
| 500 MHz to 20 GHz                                                |                                                          | +20 dBm                           |
| 20 to 40 GHz                                                     |                                                          | +16 dBm                           |
| 40 to 50 GHz                                                     |                                                          | +15 dBm                           |
| <b>Third Order Intercept - Tone spacing from 20 MHz - 50 MHz</b> |                                                          |                                   |
|                                                                  |                                                          | <b>Typical</b>                    |

|                                                                    |               |         |
|--------------------------------------------------------------------|---------------|---------|
| 10 MHz to 500 MHz                                                  |               | +26 dBm |
| 500 MHz to 20 GHz                                                  |               | +26 dBm |
| 20 to 40 GHz                                                       |               | +20 dBm |
| 40 to 50 GHz                                                       |               | +19 dBm |
| <b>Trace Noise Magnitude</b>                                       |               |         |
| 1 kHz IF bandwidth. Ratio measurement, nominal power at test port. |               |         |
| 10 MHz to 45 MHz <sup>b</sup>                                      | <0.050 dB rms |         |
| 45 MHz to 500 MHz <sup>e</sup>                                     | <0.010 dB rms |         |
| 500 MHz to 20 GHz                                                  | <0.006 dB rms |         |
| 20 GHz to 40 GHz                                                   | <0.006 dB rms |         |
| 40 GHz to 50 GHz                                                   | <0.006 dB rms |         |
| <b>Trace Noise Magnitude - Option 080 enabled<sup>b,d</sup></b>    |               |         |
| 1 kHz IF bandwidth. Ratio measurement, nominal power at test port. |               |         |
| 10 MHz to 45 MHz <sup>b</sup>                                      | <0.060 dB rms |         |
| 45 MHz to 500 MHz <sup>e</sup>                                     | <0.010 dB rms |         |
| 500 MHz to 20 GHz                                                  | <0.006 dB rms |         |
| 20 GHz to 40 GHz                                                   | <0.007 dB rms |         |
| 40 GHz to 50 GHz                                                   | <0.008 dB rms |         |
| <b>Trace Noise Phase</b>                                           |               |         |
| 1 kHz IF bandwidth. Ratio measurement, nominal power at test port. |               |         |



|                                                                    |             |  |
|--------------------------------------------------------------------|-------------|--|
| 10 MHz to<br>45 MHz <sup>b</sup>                                   | <0.350° rms |  |
| 45 MHz to<br>500 MHz                                               | <0.100° rms |  |
| 500 MHz to<br>20 GHz                                               | <0.060° rms |  |
| 20 GHz to<br>40 GHz                                                | <0.100° rms |  |
| 40 GHz to<br>50 GHz                                                | <0.100° rms |  |
| <b>Trace Noise Phase - Option 080 enabled<sup>b,d</sup></b>        |             |  |
| 1 kHz IF bandwidth. Ratio measurement, nominal power at test port. |             |  |
| 10 MHz to<br>45 MHz                                                | <0.350° rms |  |
| 45 MHz to<br>500 MHz <sup>e</sup>                                  | <0.100° rms |  |
| 500 MHz to<br>20 GHz                                               | <0.060° rms |  |
| 20 GHz to<br>40 GHz                                                | <0.100° rms |  |
| 40 GHz to<br>50 GHz                                                | <0.100° rms |  |
| <b>Reference Level Magnitude</b>                                   |             |  |
| Range                                                              | +/-200 dB   |  |
| Resolution                                                         | 0.001 dB    |  |
| <b>Reference Level Phase</b>                                       |             |  |
| Range                                                              | +/-500°     |  |
| Resolution                                                         | 0.01°       |  |
| <b>Stability Magnitude<sup>d</sup></b>                             |             |  |
| Typical ratio measurement, made at the test port.                  |             |  |

|                                                       |  |  |  |  |                                     |
|-------------------------------------------------------|--|--|--|--|-------------------------------------|
| 10 MHz to<br>45 MHz                                   |  |  |  |  | +/-0.05 dB/°C                       |
| 45 MHz to<br>20 GHz                                   |  |  |  |  | +/-0.02 dB/°C                       |
| 20 GHz to<br>40 GHz                                   |  |  |  |  | +/-0.03 dB/°C                       |
| 40 GHz to<br>50 GHz                                   |  |  |  |  | +/-0.04 dB/°C                       |
| <b>Stability Phase<sup>d</sup></b>                    |  |  |  |  |                                     |
| Typical ratio measurement, measured at the test port. |  |  |  |  |                                     |
| 10 MHz to<br>45 MHz                                   |  |  |  |  | +/-0.5°/°C                          |
| 45 MHz to<br>20 GHz                                   |  |  |  |  | +/-0.2°/°C                          |
| 20 GHz to<br>40 GHz                                   |  |  |  |  | +/-0.5°/°C                          |
| 40 GHz to<br>50 GHz                                   |  |  |  |  | +/-0.8°/°C                          |
| <b>Damage Input Level</b>                             |  |  |  |  |                                     |
| Test Port 1<br>and 2                                  |  |  |  |  | +30 dBm or<br>+/-40 VDC,<br>typical |
| R1, R2 in                                             |  |  |  |  | +15 dBm or<br>+/-15 VDC,<br>typical |
| A, B in                                               |  |  |  |  | +15 dBm or<br>+/-15 VDC,<br>typical |
| Coupler Thru<br>(Option 014 or<br>UNL/014)            |  |  |  |  | +30 dBm or<br>+/-40 VDC,<br>typical |
| Coupler Arm<br>(Option 014 or<br>UNL/014)             |  |  |  |  | +30 dBm or<br>+/-7 VDC,<br>typical  |

aTotal average (rms) noise power calculated as the mean value of a linear magnitude trace expressed in dBm.

bTypical performance.

cNoise floor may be degraded by 10 dB at particular frequencies (multiples of 5 MHz) due to spurious receiver residuals.

d0 Hz offset

eTrace noise magnitude may be degraded to 20 mdB rms at harmonic frequencies of the first IF (8.33 MHz) below 80 MHz.


fStability is defined as a ratio measurement made at the test port.

g This compression level comes from the dynamic accuracy curve with -30 dBm reference test port power.


**Table 36. Dynamic Accuracy (Specification<sup>a</sup>)**

Accuracy of the test port input power reading relative to the reference input power level.

### Magnitude\*

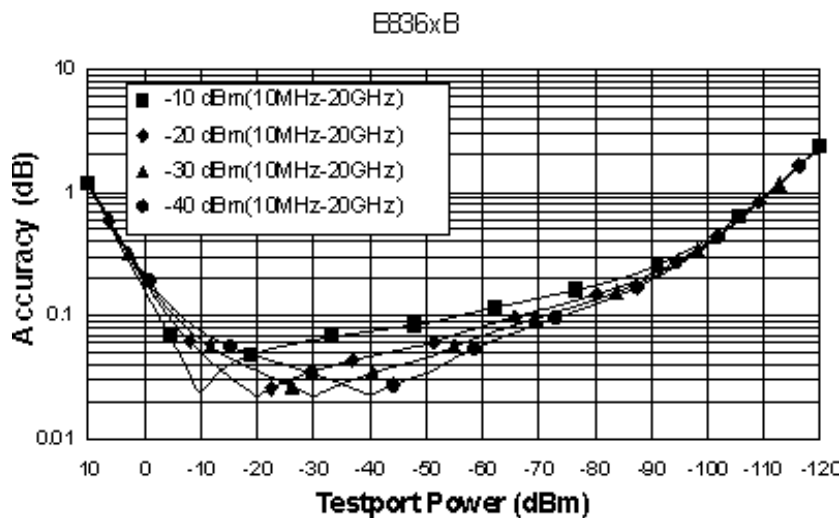


### Phase\*

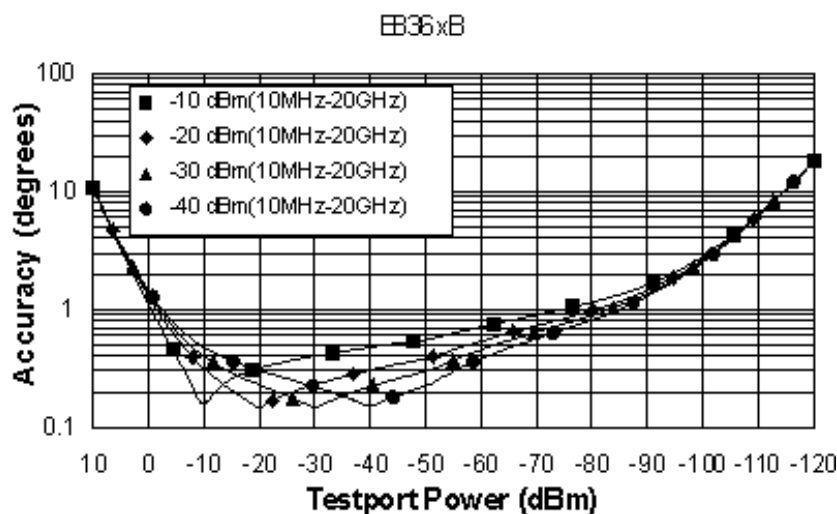


\*Below 800 MHz the coupling factor rolls off 20 dB per decade causing a shift in the dynamic accuracy curves. Please see the Uncertainty Calculator ([http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator)) for detailed compression values.


### Magnitude

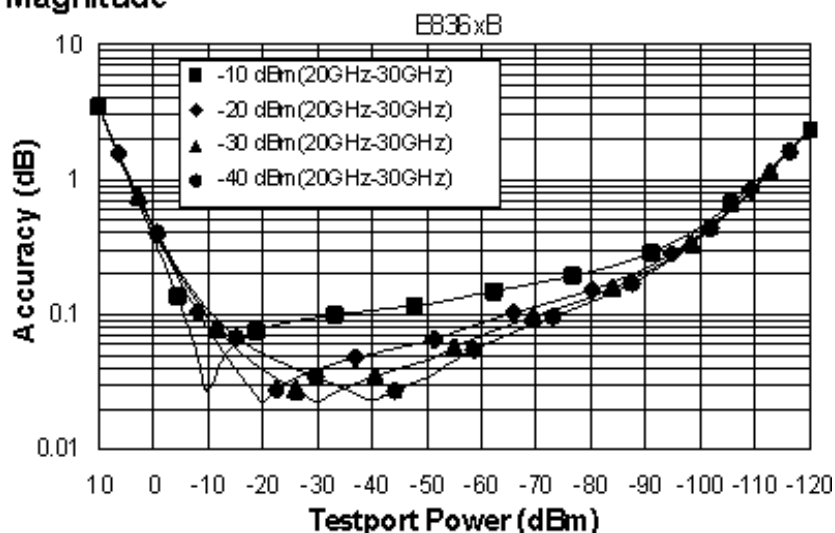


### Phase

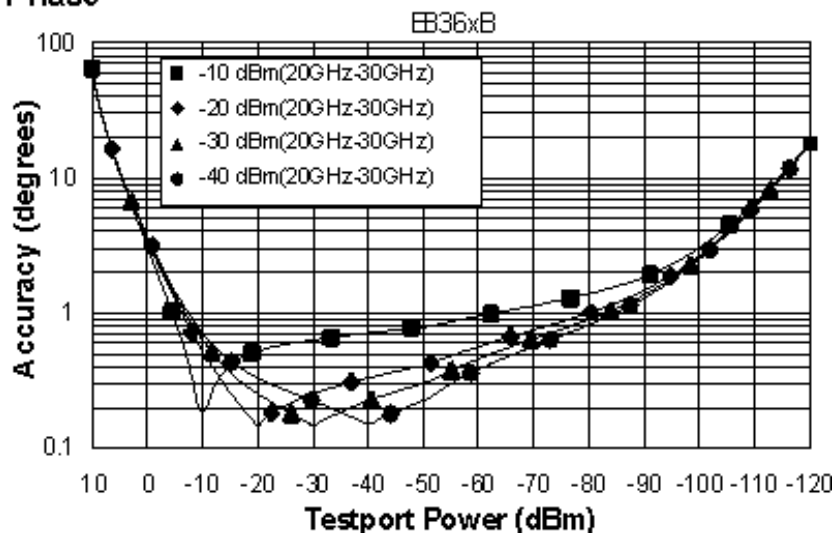


### Magnitude

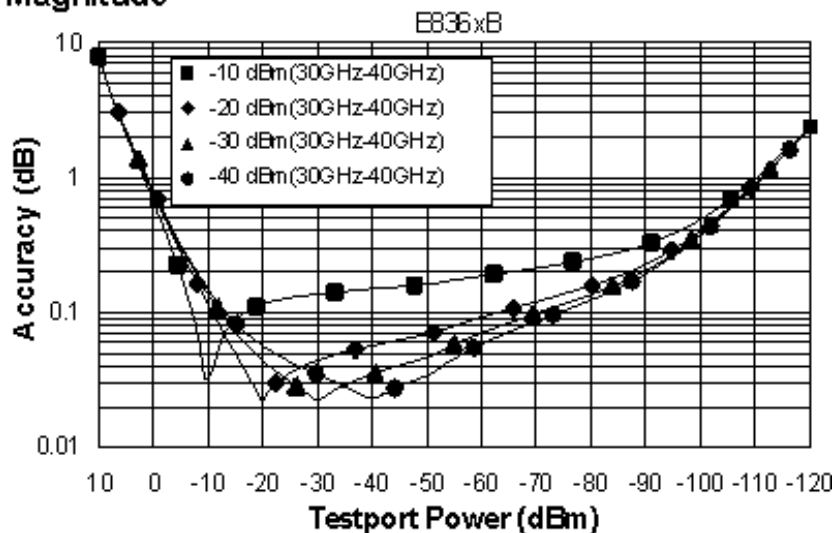


### Phase

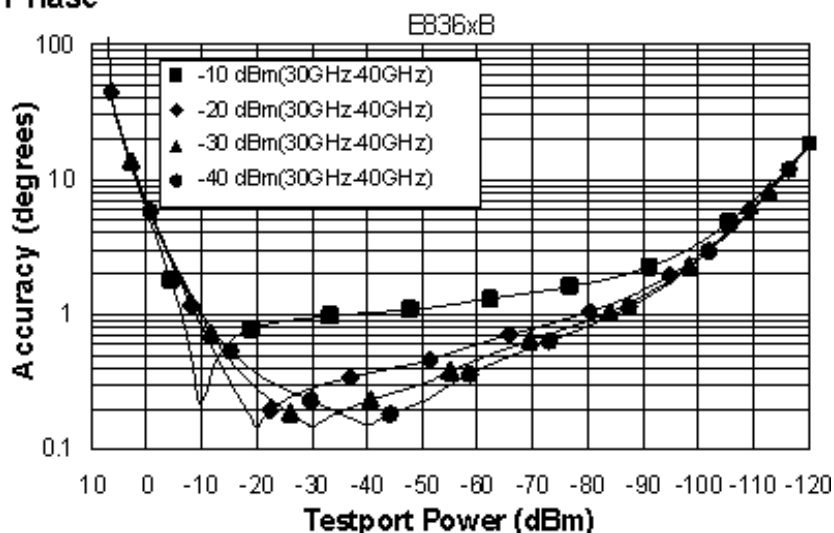

### Magnitude

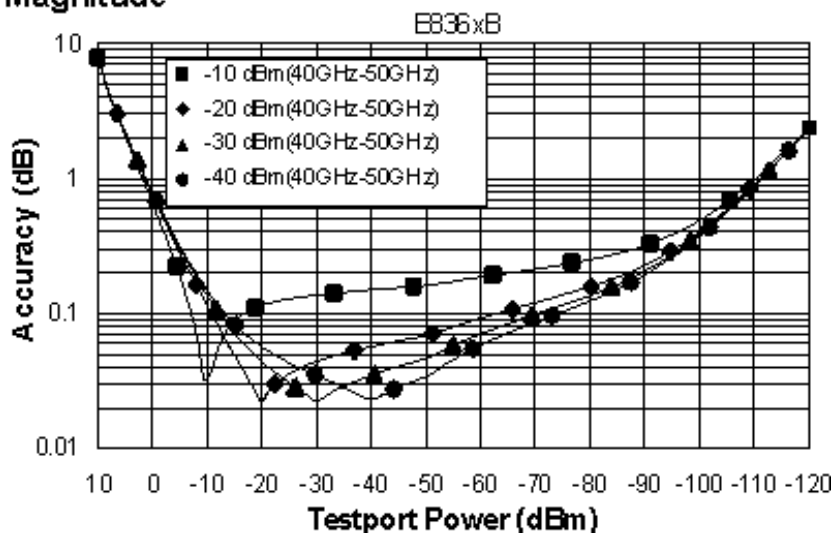

### Phase

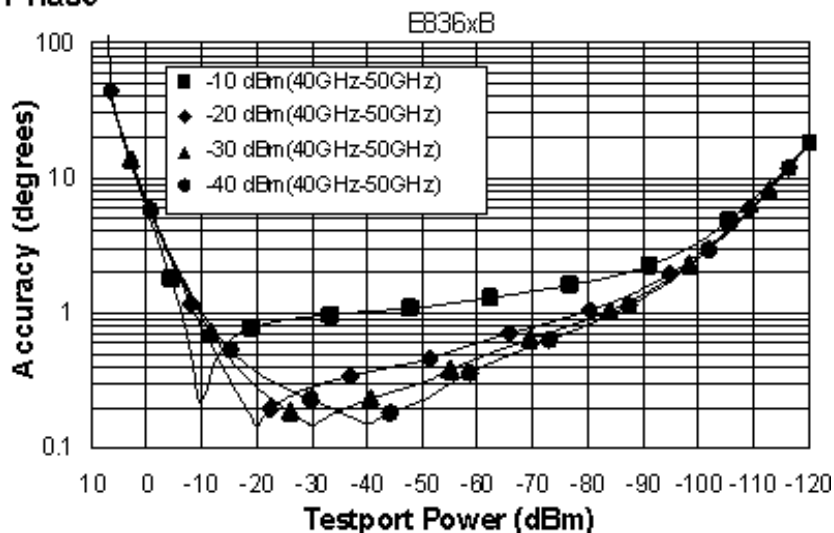


<sup>a</sup> Dynamic accuracy is verified with the following measurements:

- Compression over frequency.
- IF linearity at a single frequency of 1.195 GHz and a reference level of -20 dBm for an input power range of 0 to -120 dBm.

**Table 37. Test Port Input (Group Delay)<sup>a</sup>**

| Description           | Specification | Supplemental Information (typ.)                                                      |
|-----------------------|---------------|--------------------------------------------------------------------------------------|
| Aperture (selectable) |               | (frequency span)/(number of points -1)                                               |
| Maximum Aperture      |               | 20% of frequency span                                                                |
| Range                 |               | 0.5 x (1/minimum aperture)                                                           |
| Maximum Delay         |               | Limited to measuring no more than 180° of phase change within the minimum aperture.) |
| Accuracy              |               | See graph below. Char.                                                               |

The following graph shows characteristic group delay accuracy with full 2-port calibration and a 10 Hz IF bandwidth. Insertion loss is assumed to be < 2 dB and electrical length to be ten meters.

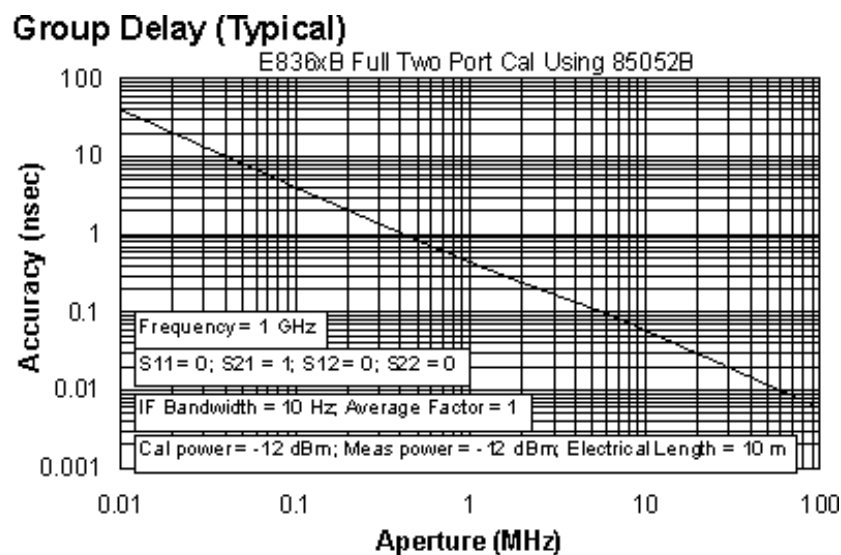

In general, the following formula can be used to determine the accuracy, in seconds, of specific group delay measurement:

$$\pm \text{Phase Accuracy (deg)} / [360 \times \text{Aperture (Hz)}]$$

Depending on the aperture and device length, the phase accuracy used is either incremental phase accuracy or worst case phase accuracy.

<sup>a</sup> Group delay is computed by measuring the phase change within a specified frequency step (determined by the frequency span and the number of points per sweep).

## General Information

### Miscellaneous Information

#### Front Panel

#### Rear Panel

#### Environment and Dimensions

**Table 38. Miscellaneous Information**

| Description               | Specification | Supplemental Information    |
|---------------------------|---------------|-----------------------------|
| System IF Bandwidth Range |               | 1 Hz to 40 kHz, nominal     |
| CPU                       |               | Intel® 500 MHz Pentium® III |

**Table 39.** Front Panel Information

| Description               | Supplemental Information                                                                                                                                          |
|---------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>RF Connectors</b>      |                                                                                                                                                                   |
| <b>E8362B</b>             |                                                                                                                                                                   |
| Type                      | 3.5 mm (male), 50 ohm, (nominal)                                                                                                                                  |
| Center Pin Recession      | 0.002 in. (characteristic)                                                                                                                                        |
| <b>E8363/4B</b>           |                                                                                                                                                                   |
| Type                      | 2.4 mm (male), 50 ohm, (nominal)                                                                                                                                  |
| Center Pin Recession      | 0.002 in. (characteristic)                                                                                                                                        |
| <b>Display</b>            |                                                                                                                                                                   |
| Size                      | 21.3 cm (8.4 in) diagonal color active matrix LCD; 640 (horizontal) X 480 (vertical) resolution; 59.83 Hz vertical refresh rate; 31.41 Hz horizontal refresh rate |
| Refresh Rate              | Vertical 59.83 Hz; Horizontal 31.41 kHz                                                                                                                           |
| <b>Display Range</b>      |                                                                                                                                                                   |
| Magnitude                 | ±200 dB (at 20 dB/div), max                                                                                                                                       |
| Phase                     | ±500°, max                                                                                                                                                        |
| Polar                     | 10 pUnits, min<br>1000 Units, max                                                                                                                                 |
| <b>Display Resolution</b> |                                                                                                                                                                   |
| Magnitude                 | 0.001 dB/div, min                                                                                                                                                 |
| Phase                     | 0.01°/div, min                                                                                                                                                    |
| <b>Marker Resolution</b>  |                                                                                                                                                                   |
| Magnitude                 | 0.001 dB, min                                                                                                                                                     |
| Phase                     | 0.01°, min                                                                                                                                                        |
| Polar                     | 0.01 mUnit, min; 0.01°, min                                                                                                                                       |

**Table 40.** Rear Panel Information

| Description                | Supplemental Information |
|----------------------------|--------------------------|
| <b>10 MHz Reference In</b> |                          |

|                                                             |                                                                              |
|-------------------------------------------------------------|------------------------------------------------------------------------------|
| Connector                                                   | BNC, female                                                                  |
| Input Frequency                                             | 10 MHz $\pm$ 10 ppm, typical                                                 |
| Input Level                                                 | -15 dBm to +20 dBm, typical                                                  |
| Input Impedance                                             | 200 $\Omega$ , nom.                                                          |
| <b>10 MHz Reference Out</b>                                 |                                                                              |
| Connector                                                   | BNC, female                                                                  |
| Output Frequency                                            | 10 MHz $\pm$ 1 ppm, typical                                                  |
| Signal Type                                                 | Sine Wave, typical                                                           |
| Output Level                                                | +10 dBm $\pm$ 4 dB into 50 $\Omega$ , typical                                |
| Output Impedance                                            | 50 $\Omega$ , nominal                                                        |
| Harmonics                                                   | <-40 dBc, typical                                                            |
| <b>Option H08 &amp; H11 Rear Panel Connectors (typical)</b> |                                                                              |
| IF Connectors                                               | A, R1, R2, B (BNC Connectors)                                                |
| IF Connector Input Frequency                                | 8 1/3 MHz                                                                    |
| Nominal Input Impedance at IF Inputs                        | 50 $\Omega$                                                                  |
| RF Damage Level to IF Connector Inputs                      | -20.0 dBm                                                                    |
| DC Damage Level to IF Connector Inputs                      | 25 volts                                                                     |
| 0.1 dB Compression Point at IF Inputs                       | -27.0 dBm                                                                    |
| Pulse Input Connectors <sup>1</sup>                         | A, R1, R2, B (BNC Connectors)                                                |
| Nominal Input Impedance at Pulse Inputs                     | 1 Kohm                                                                       |
| Minimum IF Gate Width                                       | 20 ns for less than 1 dB deviation from theoretical performance <sup>2</sup> |
| DC Damage Level to Pulse Connector Inputs                   | 5.5 volts                                                                    |
| Drive Voltage                                               | TTL (0, +5.0) Volts                                                          |
| <b>Rear Panel LO Power (Typical)</b>                        |                                                                              |



|                                                  |                                                                                                                                                                                                                    |
|--------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1.7 GHz- 20 GHz                                  | -7 to -16 dBm                                                                                                                                                                                                      |
| <b>Rear Panel RF Power 8362B (Typical)</b>       |                                                                                                                                                                                                                    |
| 1.7 GHz to 20 GHz                                | -5 to 16 dBm (at 5 dBm test port power <sup>3</sup> )                                                                                                                                                              |
| <b>Rear Panel RF Power 8363B/8364B (Typical)</b> |                                                                                                                                                                                                                    |
| 1.7 GHz to 10 GHz                                | -2 to 12 dBm (at 5 dBm test port power <sup>3</sup> )                                                                                                                                                              |
| 10 GHz to 16 GHz                                 | 0 to 8 dBm (at 5 dBm test port power <sup>3</sup> )                                                                                                                                                                |
| 16 GHz to 20 GHz                                 | +5 to 1 dBm (at 5 dBm test port power <sup>3</sup> )                                                                                                                                                               |
| <b>VGA Video Output</b>                          |                                                                                                                                                                                                                    |
| Connector                                        | 15-pin mini D-Sub; Drives VGA compatible monitors                                                                                                                                                                  |
| Devices Supported:                               |                                                                                                                                                                                                                    |
|                                                  | <b>Resolutions:</b>                                                                                                                                                                                                |
| Flat Panel (TFT)                                 | 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                                   |
| Flat Panel (DSTN)                                | 800 X 600, 640 X 480                                                                                                                                                                                               |
| CRT Monitor                                      | 1280 X 1024, 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                      |
|                                                  | Simultaneous operation of the internal and external displays is allowed, but with 640 X 480 resolution only. If you change resolution, you can only view the external display (internal display will "white out"). |
| <b>Bias Input Connectors (Option UNL)</b>        |                                                                                                                                                                                                                    |
| Bias current                                     | 500 mA, maximum                                                                                                                                                                                                    |
| Bias voltage                                     | 40 Volts, maximum                                                                                                                                                                                                  |
| <b>Test Set IO</b>                               |                                                                                                                                                                                                                    |
|                                                  | 25-pin D-Sub connector, available for external test set control.                                                                                                                                                   |
| <b>Aux IO</b>                                    |                                                                                                                                                                                                                    |
|                                                  | 25-pin D-Sub connector, male, analog and digital IO.                                                                                                                                                               |
| <b>Handler IO</b>                                |                                                                                                                                                                                                                    |
|                                                  | 36-pin parallel I/O port; all input/output signals are default set to negative logic; can be reset to positive logic via GPIB command.                                                                             |
| <b>GPIB</b>                                      |                                                                                                                                                                                                                    |
|                                                  | 24-pin D-sub (Type D-24), female; compatible with IEEE-488.                                                                                                                                                        |
| <b>Parallel Port (LPT1)</b>                      |                                                                                                                                                                                                                    |

|                               |                                                                                                                                                      |
|-------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------|
|                               | 25-pin D-Sub miniature connector, female; provides connection to printers or any other parallel port peripherals                                     |
| <b>Serial Port (COM 1)</b>    |                                                                                                                                                      |
|                               | 9-pin D-Sub, male; compatible with RS-232                                                                                                            |
| <b>USB Port</b>               |                                                                                                                                                      |
|                               | One port on front panel and five ports on rear panel. Universal Serial Bus jack, Type A configuration (4 contacts inline, contact 1 on left); female |
| Contact 1                     | Vcc: 4.75 to 5.25 VDC, 500 mA, maximum                                                                                                               |
| Contact 2                     | -Data                                                                                                                                                |
| Contact 3                     | +Data                                                                                                                                                |
| Contact 4                     | Ground                                                                                                                                               |
| <b>LAN</b>                    |                                                                                                                                                      |
|                               | 10/100BaseT Ethernet, 8-pin configuration; auto selects between the two data rates                                                                   |
| <b>Line Power<sup>4</sup></b> |                                                                                                                                                      |
| Frequency                     | 48 Hz to 66 Hz                                                                                                                                       |
| Voltage at 115 V Setting      | 90 to 132 VAC; 120 VAC, nominal                                                                                                                      |
| Voltage at 220 V Setting      | 198 to 264 VAC; 240 VAC, nominal                                                                                                                     |
| VA Max                        | 600 VA maximum                                                                                                                                       |

1 Pulse input connectors are operational only with Option H08 (Pulse Measurement Capability) enabled.

2 Based on deviation from signal reduction equation:  $\text{Signal Reduction (dB)} = 20\log_{10}(\text{Duty\_cycle}) = 20\log_{10}(\text{pulse\_width/period})$ . Measured at Pulse Repetition Frequency (PFR) of 1 MHz.

3 Test port power has to be at a high enough level such that the Drop Cal does not occur. If Drop Cal occurs then the power out of the rear panel RF connector will drop by about 15 dB.

4 A third-wire ground is required.

**Table 41.** Analyzer Environment and Dimensions

| Description                                                                 | Supplemental Information                                                                                                                                                                                |                    |                    |
|-----------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------|--------------------|
| <b>General Environmental</b>                                                |                                                                                                                                                                                                         |                    |                    |
| RFI/EMI Susceptibility                                                      | Defined by CISPR Pub. 11, Group 1, Class A, and IEC 50082-1                                                                                                                                             |                    |                    |
| ESD                                                                         | Minimize using static-safe work procedures and an antistatic bench mat                                                                                                                                  |                    |                    |
| Dust                                                                        | Minimize for optimum reliability                                                                                                                                                                        |                    |                    |
| <b>Operating Environment</b>                                                |                                                                                                                                                                                                         |                    |                    |
| Temperature                                                                 | 0 °C to +40 °C<br>Instrument powers up, phase locks, and displays no error messages within this temperature range (except for "source unleveled" error message that may occur at temperature extremes). |                    |                    |
| Error-Corrected Temperature Range                                           | 23°C ± 3°C<br>with less than 1°C deviation from calibration temp.                                                                                                                                       |                    |                    |
| Humidity                                                                    | 5% to 95% at +40 °C                                                                                                                                                                                     |                    |                    |
| Altitude                                                                    | 0 to 4500 m (14,760 ft.)                                                                                                                                                                                |                    |                    |
| <b>Non-Operating Storage Environment</b>                                    |                                                                                                                                                                                                         |                    |                    |
| Temperature                                                                 | -40 °C to +70 °C                                                                                                                                                                                        |                    |                    |
| Humidity                                                                    | 0% to 90% at +65 °C (non-condensing)                                                                                                                                                                    |                    |                    |
| Altitude                                                                    | 0 to 15,240 m (50,000 ft.)                                                                                                                                                                              |                    |                    |
| <b>Cabinet Dimensions</b>                                                   |                                                                                                                                                                                                         |                    |                    |
|                                                                             | <b>Height</b>                                                                                                                                                                                           | <b>Width</b>       | <b>Depth</b>       |
| Excluding front and rear panel hardware and feet                            | 267 mm<br>10.5 in                                                                                                                                                                                       | 426 mm<br>16.75 in | 427 mm<br>16.8 in  |
| As shipped - includes front panel connectors, rear panel bumpers, and feet. | 280 mm<br>11.0 in                                                                                                                                                                                       | 435 mm<br>17.1 in  | 470 mm<br>18.5 in  |
| As shipped plus handles                                                     | 280 mm<br>11.0 in                                                                                                                                                                                       | 458 mm<br>18 in    | 501 mm<br>19.70 in |
| As shipped plus rack-mount flanges                                          | 280 mm<br>11.0 in                                                                                                                                                                                       | 483 mm<br>19 in    | 470 mm<br>18.5 in  |
| As shipped plus handles and flanges                                         | 280 mm<br>11.0 in                                                                                                                                                                                       | 483 mm<br>19 in    | 501 mm<br>19.70 in |
| <b>Weight</b>                                                               |                                                                                                                                                                                                         |                    |                    |
| <b>Net</b>                                                                  |                                                                                                                                                                                                         |                    |                    |
| E8362B                                                                      | 28.6 kg (63.5 lb), nominal                                                                                                                                                                              |                    |                    |
| E8363/4B                                                                    | 29 kg (64 lb), nominal                                                                                                                                                                                  |                    |                    |
| <b>Shipping</b>                                                             |                                                                                                                                                                                                         |                    |                    |

|          |                            |
|----------|----------------------------|
| E8362B   | 35.8 kg (79.5 lb), nominal |
| E8363/4B | 36.3 kg 80 lb), nominal    |

## Measurement Throughput Summary

### Typical Cycle Time for Measurement Completion

#### Cycle Time vs IF Bandwidth

#### Cycle Time vs Number of Points

#### Data Transfer Time

**Table 42** Typical Cycle Time<sup>a,b</sup> (ms) for Measurement Completion

|                                                       | Number of Points |     |      |        |
|-------------------------------------------------------|------------------|-----|------|--------|
|                                                       | 201              | 401 | 1601 | 16,001 |
| <b>Start 28 GHz, Stop 30 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 12               | 19  | 55   | 503    |
| 2-Port cal                                            | 29               | 44  | 124  | 1112   |
| <b>Start 10 MHz, Stop 10 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 86               | 93  | 121  | 583    |
| 2-Port cal                                            | 179              | 199 | 267  | 1301   |
| <b>Start 10 MHz, Stop 20 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 126              | 130 | 153  | 597    |
| 2-Port cal                                            | 264              | 275 | 335  | 1321   |
| <b>Start 10 MHz, Stop 40 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 185              | 190 | 213  | 621    |
| 2-Port cal                                            | 382              | 401 | 459  | 1374   |
| <b>Start 10 MHz, Stop 50 GHz, 35 kHz IF bandwidth</b> |                  |     |      |        |
| Uncorrected,<br>1-port cal                            | 210              | 216 | 243  | 643    |
| 2-Port cal                                            | 436              | 450 | 522  | 1405   |

| <b>Start 10 MHz, Stop 67 GHz, 35 kHz IF bandwidth</b> |     |     |     |      |
|-------------------------------------------------------|-----|-----|-----|------|
| Uncorrected<br>1-Port cal                             | 244 | 254 | 300 | 645  |
| 2-Port cal                                            | 502 | 524 | 591 | 1423 |

a Typical performance.

b Includes sweep time, retrace time and band-crossing time. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S11) measurement.

**Table 43. Cycle Time vs IF Bandwidth<sup>a</sup>**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 28 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| <b>IF Bandwidth (Hz)</b> | <b>Cycle Time (ms)<sup>b</sup></b> | <b>Cycle Time (ms)<br/>Option 080<br/>enabled</b> |
|--------------------------|------------------------------------|---------------------------------------------------|
| 40,000                   | 11                                 | 100                                               |
| 35,000                   | 12                                 | 101                                               |
| 30,000                   | 13                                 | 102                                               |
| 20,000                   | 16                                 | 106                                               |
| 10,000                   | 30                                 | 127                                               |
| 7000                     | 38                                 | 138                                               |
| 5000                     | 50                                 | 152                                               |
| 3000                     | 74                                 | 182                                               |
| 1000                     | 274                                | 326                                               |
| 300                      | 694                                | 782                                               |
| 100                      | 1905                               | 2054                                              |
| 30                       | 6091                               | 6355                                              |
| 10                       | 17916                              | 18372                                             |

a Typical performance.

b Cycle time includes sweep and retrace time.

**Table 44. Cycle Time vs Number of Points<sup>a</sup>**

Applies to the Preset condition (35 kHz IF bandwidth, correction off) except for the following changes:

- CF = 28 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Number of Points | Cycle Time (ms) <sup>b</sup> |
|------------------|------------------------------|
| 3                | 6                            |
| 11               | 6                            |
| 51               | 7                            |
| 101              | 9                            |
| 201              | 12                           |
| 401              | 18                           |
| 801              | 30                           |
| 1601             | 55                           |
| 16,001           | 497                          |

a Typical performance.

b Cycle time includes sweep and retrace time.

**Table 45. Data Transfer Time (ms)<sup>a</sup>**

|                                               | Number of Points |     |      |        |
|-----------------------------------------------|------------------|-----|------|--------|
|                                               | 201              | 401 | 1601 | 16,001 |
| <b>SCPI over GPIB</b>                         |                  |     |      |        |
| <b>(program executed on external PC)</b>      |                  |     |      |        |
| 32-bit floating point                         | 7                | 12  | 43   | 435    |
| 64-bit floating point                         | 12               | 22  | 84   | 856    |
| ASCII                                         | 64               | 124 | 489  | 5054   |
| <b>SCPI</b>                                   |                  |     |      |        |
| <b>(program executed in the analyzer)</b>     |                  |     |      |        |
| 32-bit floating point                         | 1                | 2   | 3    | 30     |
| 64-bit floating point                         | 2                | 2   | 4    | 40     |
| ASCII                                         | 29               | 56  | 222  | 2220   |
| <b>COM (program executed in the analyzer)</b> |                  |     |      |        |
| 32-bit floating point                         | 1                | 1   | 1    | 6      |
| Variant type                                  | 1                | 2   | 6    | 68     |

## DCOM over LAN

(program executed on external PC)


|                       |   |   |    |     |
|-----------------------|---|---|----|-----|
| 32-bit floating point | 1 | 1 | 2  | 121 |
| Variant type          | 3 | 6 | 19 | 939 |

a Typical performance


**Note:** Specifications for Recall & Sweep Speed are not provided for the E836xB analyzers.

## Test Set Block Diagrams


E836xB - Standard Configuration and Standard Power Range

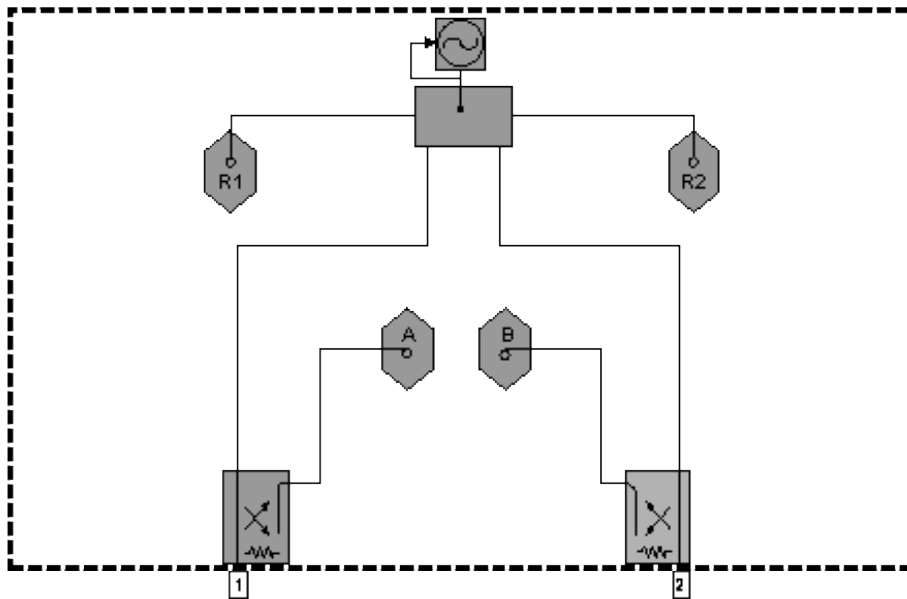

E836xB - Option UNL Standard Configuration with Extended Power Range and Bias - Tees

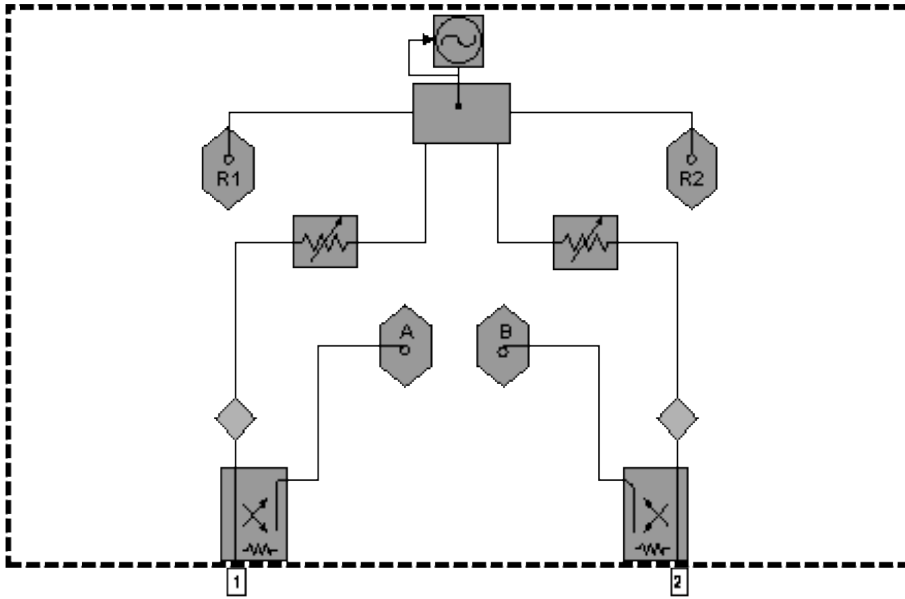


E836xB - Option UNL Standard Configuration with Extended Power Range and Bias - Tees, and Option 016, Receiver Attenuators

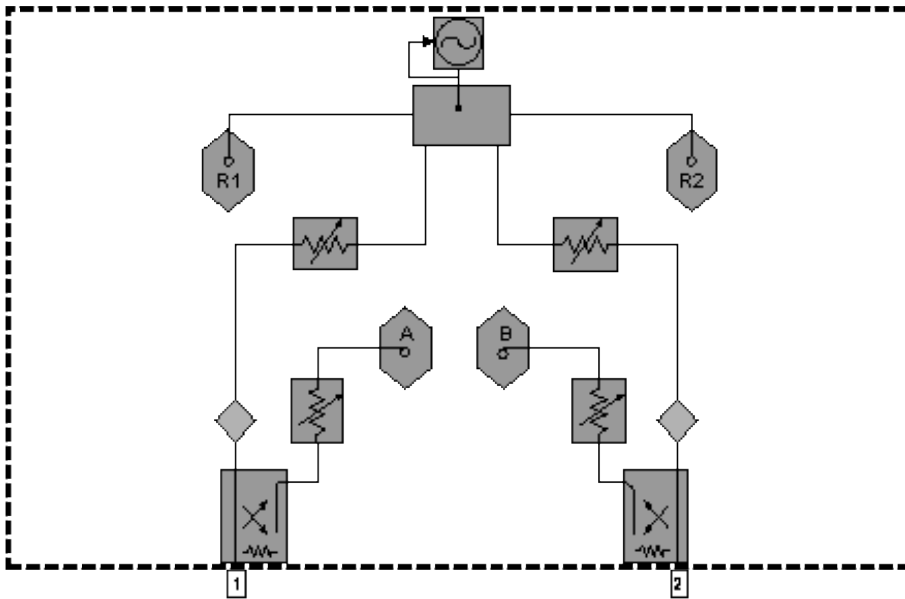

**Test Set with Option 014 Block Diagrams**


E836xB - Option 014 – Configurable Test Set and Standard Power Range



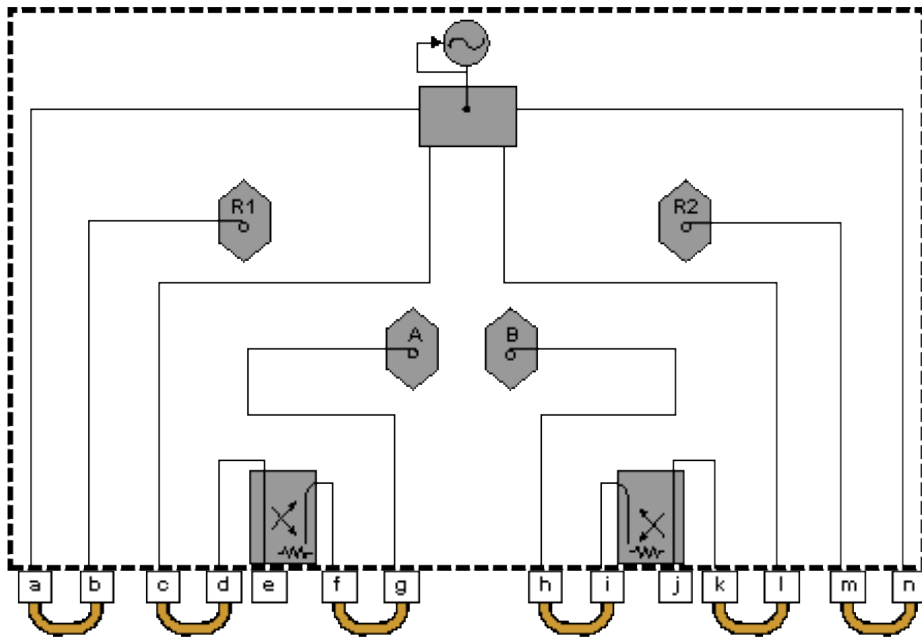


| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

E836xB - Option 014 – Configurable Test Set and Standard Power Range, and Option 081 Reference Channel Transfer Switch

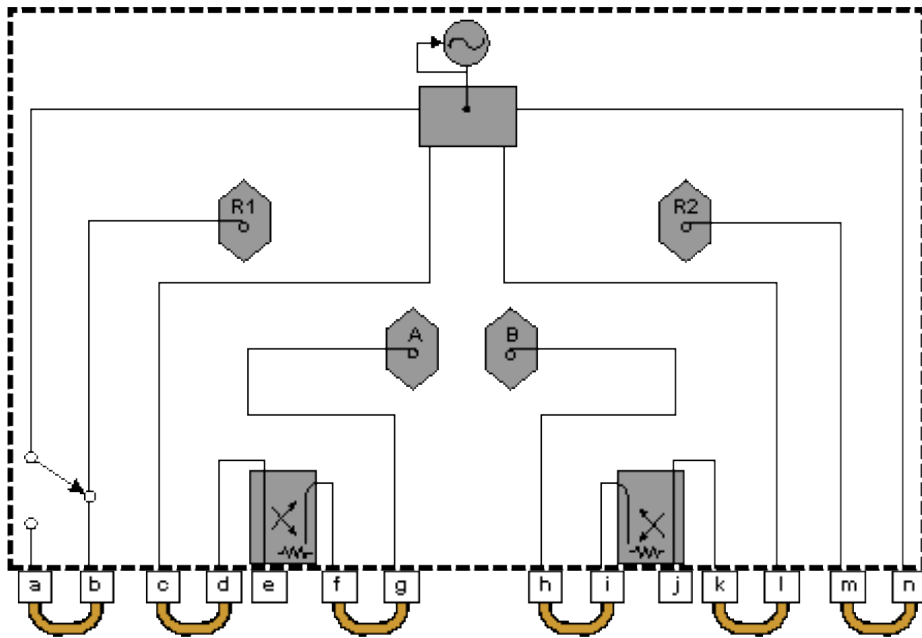


| Item     | Description | Item     | Description |
|----------|-------------|----------|-------------|
| <b>a</b> | SOURCE OUT  | <b>h</b> | RCVR B IN   |
| <b>b</b> | RCVR R1 IN  | <b>i</b> | CPLR ARM    |
| <b>c</b> | SOURCE OUT  | <b>j</b> | PORT 2      |
| <b>d</b> | CPLR THRU   | <b>k</b> | CPLR THRU   |
| <b>e</b> | PORT 1      | <b>l</b> | SOURCE OUT  |
| <b>f</b> | CPLR ARM    | <b>m</b> | RCVR R2 IN  |
| <b>g</b> | RCVR A IN   | <b>n</b> | SOURCE OUT  |

E836xB - Option 014 Configurable Test Set, and Option UNL Extended Power Range and Bias - Tees

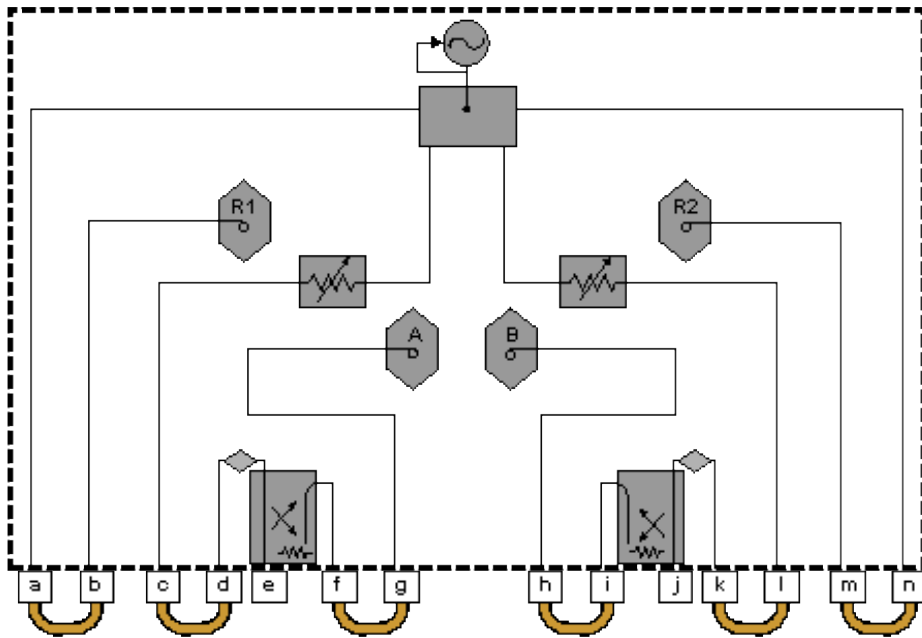


| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

E836xB - Option 014 Configurable Test Set, and Option UNL Extended Power Range and Bias - Tees, and Option 081 Reference Channel Transfer Switch

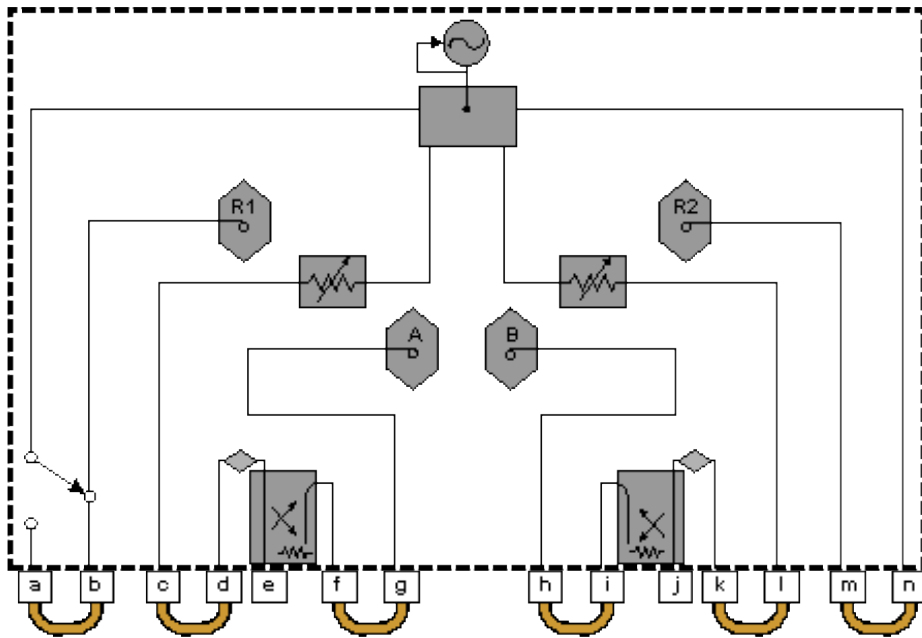


| Item     | Description | Item     | Description |
|----------|-------------|----------|-------------|
| <b>a</b> | SOURCE OUT  | <b>h</b> | RCVR B IN   |
| <b>b</b> | RCVR R1 IN  | <b>i</b> | CPLR ARM    |
| <b>c</b> | SOURCE OUT  | <b>j</b> | PORT 2      |
| <b>d</b> | CPLR THRU   | <b>k</b> | CPLR THRU   |
| <b>e</b> | PORT 1      | <b>l</b> | SOURCE OUT  |
| <b>f</b> | CPLR ARM    | <b>m</b> | RCVR R2 IN  |
| <b>g</b> | RCVR A IN   | <b>n</b> | SOURCE OUT  |

E836xB - Option 014 Configurable Test Set and Option UNL, Extended Power Range and Bias - Tees and Option 016 Receiver Attenuators

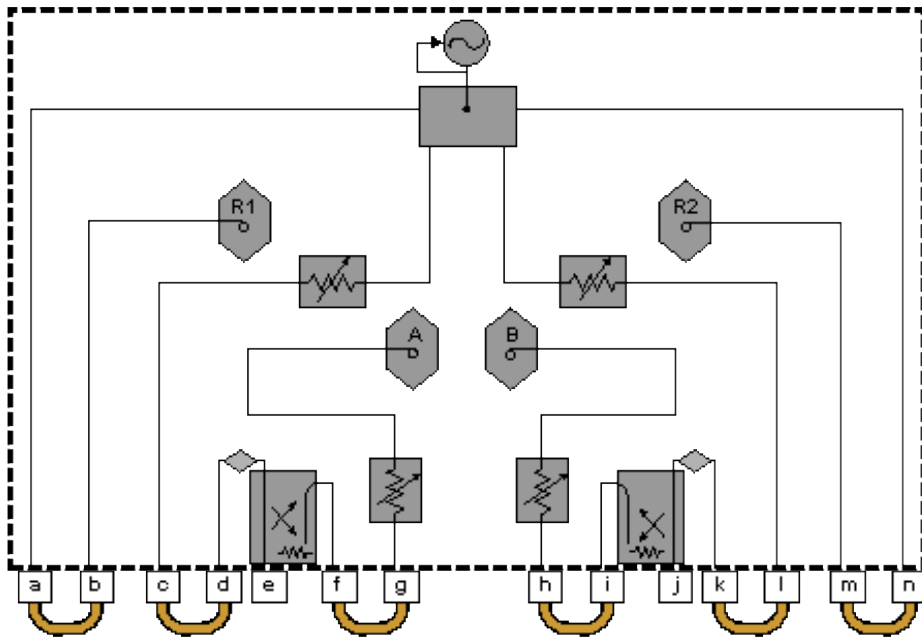

| Item     | Description | Item     | Description |
|----------|-------------|----------|-------------|
| <b>a</b> | SOURCE OUT  | <b>h</b> | RCVR B IN   |
| <b>b</b> | RCVR R1 IN  | <b>i</b> | CPLR ARM    |
| <b>c</b> | SOURCE OUT  | <b>j</b> | PORT 2      |
| <b>d</b> | CPLR THRU   | <b>k</b> | CPLR THRU   |
| <b>e</b> | PORT 1      | <b>l</b> | SOURCE OUT  |
| <b>f</b> | CPLR ARM    | <b>m</b> | RCVR R2 IN  |
| <b>g</b> | RCVR A IN   | <b>n</b> | SOURCE OUT  |

E836xB - Option 014 Configurable Test Set, and Option UNL Extended Power Range and Bias - Tees, and Option 016 Receiver Attenuators, and Option 081 Reference Channel Transfer Switch

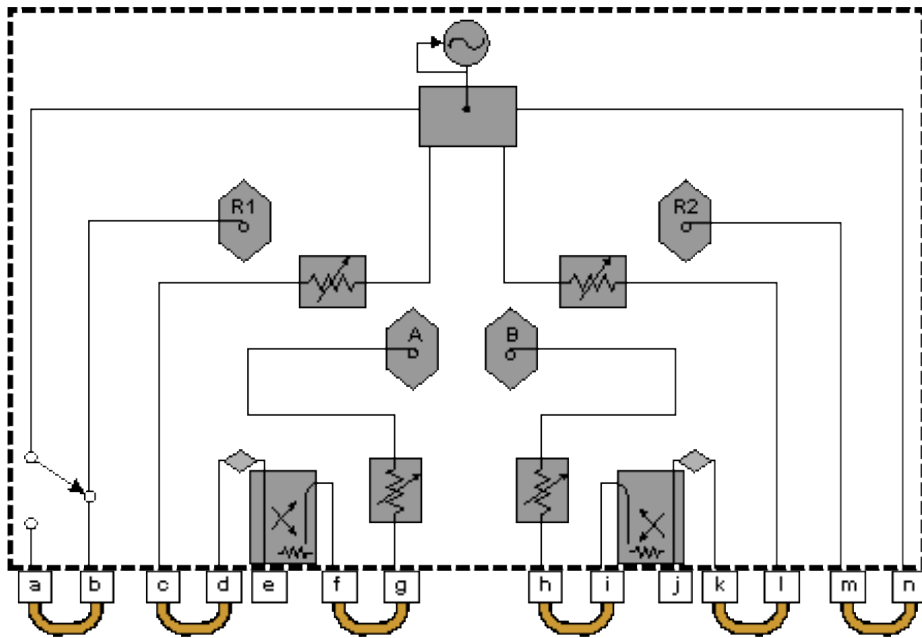

| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

## Technical Specifications for the N5230A

### Options 020/025, 120/125, 220/225, 420/425, or 520/525 (2-Port PNA)

(Rev. 2005-06-01)

---

This is a complete list of the N5230A Options 020, 025, 120, 125, 220, 225, 420, 425, 520, or 525 network analyzer technical specifications.

- To optimize viewing of uncertainty curves, click the Maximize button.
  - To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "N5230A Specifications"
  - This N5230A document provides technical specifications for the 85056A 2.4 mm, 85052B 3.5 mm, and 85032B Type-N calibration kits and the N4691A, and N4693A ECal modules. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your calibration kit and PNA setup.
- 

#### Definitions

#### Corrected System Performance

##### System Dynamic Range

##### Extended Dynamic Range

##### 3.5mm Connectors

##### 2.4mm Connectors

##### Type-N Connectors

#### Uncorrected System Performance

#### Test Port Output

#### Test Port Input

#### Dynamic Accuracy

#### Group Delay

#### General Information

#### Measurement Throughput Summary

#### Front-panel Jumper Specs (Options 025, 125, 225, 425, 525)

#### Option 020, or 120, or 220, or 420, or 520 (Standard Test Set and Standard Power Range) Analyzer Block Diagram

#### Option 025, or 125, or 225, or 425, or 525 (Configurable Test Set and Extended Power Range) Analyzer Block Diagram

## Definitions

All specifications and characteristics apply over a 25 °C  $\pm$ 5 °C range (unless otherwise stated) and 90 minutes after the instrument has been turned on.

**Specification (spec.):** Warranted performance. Specifications include guardbands to account for the expected statistical performance distribution, measurement uncertainties, and changes in performance due to environmental conditions.

**Characteristic (char.):** A performance parameter that the product is expected to meet before it leaves the factory, but that is not verified in the field and is not covered by the product warranty. A characteristic includes the same guardbands as a specification.

**Typical (typ.):** Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Nominal (nom.):** A general, descriptive term that does not imply a level of performance. It is not covered by the product warranty.

**Calibration:** The process of measuring known standards to characterize a network analyzer's systematic (repeatable) errors.

**Corrected (residual):** Indicates performance after error correction (calibration). It is determined by the quality of calibration standards and how well "known" they are, plus system repeatability, stability, and noise.

**Uncorrected (raw):** Indicates instrument performance without error correction. The uncorrected performance affects the stability of a calibration.

**Standard:** When referring to the analyzer, this includes no options unless noted otherwise.

## Corrected System Performance

The specifications in this section apply for measurements made with the N5230A analyzer with the following conditions:

- 10 Hz IF bandwidth
- No averaging applied to data
- Isolation calibration with an averaging factor of 8

[System Dynamic Range](#)

[Extended Dynamic Range](#)

[3.5mm Connectors](#)

[2.4mm Connectors](#)

[Type-N Connectors](#)

**Table 1.** System Dynamic Range<sup>1</sup>

| Description | Specification (dB) at Test Port |            |            |            | Typical (dB) at Test Port |            |            |            |
|-------------|---------------------------------|------------|------------|------------|---------------------------|------------|------------|------------|
|             | Options 020, 120                | Option 220 | Option 420 | Option 520 | Options 020, 120          | Option 220 | Option 420 | Option 520 |
|             |                                 |            |            |            |                           |            |            |            |



| Standard Configuration and Standard Power Range |     |     |     |     |    |     |    |    |
|-------------------------------------------------|-----|-----|-----|-----|----|-----|----|----|
| 300 kHz to 1 MHz                                | 103 | --  | --  | --  | -- | --  | -- | -- |
| 1 MHz to 10 MHz                                 | 113 | --  | --  | --  | -- | --  | -- | -- |
| 10 MHz to 45 MHz                                | 122 | --  | --  | --  | -- | 103 | 89 | 89 |
| 45 MHz to 500 MHz <sup>2</sup>                  | 122 | 105 | 90  | 90  | -- | --  | -- | -- |
| 500 MHz to 2 GHz                                | 122 | 110 | 110 | 110 | -- | --  | -- | -- |
| 2 GHz to 6 GHz                                  | 122 | 110 | 110 | 110 | -- | --  | -- | -- |
| 6 GHz to 8 GHz                                  | 120 | 110 | 110 | 110 | -- | --  | -- | -- |
| 8 GHz to 9 GHz                                  | 120 | 110 | 100 | 100 | -- | --  | -- | -- |
| 9 GHz to 10.5 GHz                               | 116 | 110 | 100 | 100 | -- | --  | -- | -- |
| 10.5 GHz to 12.5 GHz                            | 111 | 110 | 100 | 100 | -- | --  | -- | -- |
| 12.5 GHz to 13.5 GHz                            | 109 | 108 | 100 | 100 | -- | --  | -- | -- |
| 13.5 GHz to 20 GHz                              | --  | 108 | 100 | 100 | -- | --  | -- | -- |
| 20 GHz to 31.25 GHz                             | --  | --  | 95  | 95  | -- | --  | -- | -- |
| 31.25 GHz to 40 GHz                             | --  | --  | 90  | 90  | -- | --  | -- | -- |
| 40 GHz to 50 GHz                                | --  | --  | --  | 79  | -- | --  | -- | -- |

**Table 1.** System Dynamic Range<sup>1</sup> (Continued)

| Description                                           | Specification (dB) at Test Port |            |            |            | Typical (dB) at Test Port |            |            |            |
|-------------------------------------------------------|---------------------------------|------------|------------|------------|---------------------------|------------|------------|------------|
|                                                       | Options 025, 125                | Option 225 | Option 425 | Option 525 | Options 025, 125          | Option 225 | Option 425 | Option 525 |
| <b>Configurable Test Set and Extended Power Range</b> |                                 |            |            |            |                           |            |            |            |
| 300 KHz to 1 MHz                                      | 102                             | --         | --         | --         | --                        | --         | --         | --         |
| 1 MHz to 10 MHz                                       | 112                             | --         | --         | --         | --                        | --         | --         | --         |

|                                |     |     |     |     |    |     |    |    |
|--------------------------------|-----|-----|-----|-----|----|-----|----|----|
| 10 MHz to 45 MHz               | 121 | --  | --  | --  | -- | 103 | 88 | 88 |
| 45 MHz to 500 MHz <sup>2</sup> | 121 | 105 | 90  | 90  | -- | --  | -- | -- |
| 500 MHz to 2 GHz               | 121 | 110 | 110 | 110 | -- | --  | -- | -- |
| 2 GHz to 6 GHz                 | 121 | 110 | 110 | 110 | -- | --  | -- | -- |
| 6 GHz to 8 GHz                 | 120 | 110 | 110 | 110 | -- | --  | -- | -- |
| 8 GHz to 9 GHz                 | 120 | 110 | 100 | 100 | -- | --  | -- | -- |
| 9 GHz to 10.5 GHz              | 116 | 110 | 100 | 100 | -- |     |    |    |
| 10.5 GHz to 12.5 GHz           | 111 | 110 | 100 | 100 | -- | --  | -- | -- |
| 12.5 GHz to 13.5 GHz           | 108 | 108 | 100 | 100 | -- | --  | -- | -- |
| 13.5 GHz to 20 GHz             | --  | 108 | 100 | 100 | -- | --  | -- | -- |
| 20 GHz to 31.25 GHz            | --  | --  | 92  | 92  | -- | --  | -- | -- |
| 31.25 GHz to 40 GHz            | --  | --  | 87  | 87  | -- | --  | -- | -- |
| 40 GHz to 50 GHz               | --  | --  | --  | 75  | -- | --  | -- | -- |

1 The system dynamic range is calculated as the difference between the noise floor and the specified source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account.

2 May be degraded by 10 dB at particular frequencies (multiples of 5 MHz) below 500 MHz due to spurious receiver residuals. Methods are available to regain the full dynamic range.

**Receiver Dynamic Range technical specifications are not provided in this N5230A specs document.**

**Table 2.** Extended Dynamic Range<sup>1</sup>

| Description                                           | Specification (dB) at Direct Receiver Access Input |            |            |            | Typical (dB) at Direct Receiver Access Input |            |            |            |
|-------------------------------------------------------|----------------------------------------------------|------------|------------|------------|----------------------------------------------|------------|------------|------------|
|                                                       | Option 025, 125                                    | Option 225 | Option 425 | Option 525 | Option 025, 125                              | Option 225 | Option 425 | Option 525 |
| <b>Configurable Test Set and Extended Power Range</b> |                                                    |            |            |            |                                              |            |            |            |
| 300 kHz to 1 MHz                                      | 118                                                | --         | --         | --         | --                                           | --         | --         | --         |
| 1 MHz to 10 MHz                                       | 128                                                | --         | --         | --         | --                                           | --         | --         | --         |
| 10 MHz to 45 MHz                                      | 137                                                | --         | --         | --         | --                                           | 115        | 109        | 109        |
| 45 MHz to 500 MHz <sup>2</sup>                        | 137                                                | 117        | 111        | 111        | --                                           | --         | --         | --         |
| 500 MHz to 2 GHz                                      | 137                                                | 122        | 122        | 122        | --                                           | --         | --         | --         |
| 2 GHz to 6 GHz                                        | 137                                                |            |            |            |                                              |            |            |            |
| 6 GHz to 8 GHz                                        | 136                                                | 122        | 122        | 122        | --                                           | --         | --         | --         |
| 8 GHz to 9 GHz                                        | 136                                                |            |            |            |                                              |            |            |            |
| 9 GHz to 10.5 GHz                                     | 132                                                | 122        | 112        | 112        | --                                           | --         | --         | --         |
| 10.5 GHz to 12.5 GHz                                  | 127                                                | 122        | 112        | 112        | --                                           | --         | --         | --         |
| 12.5 GHz to 13.5 GHz                                  | 124                                                | 120        | 112        | 112        | --                                           | --         | --         | --         |
| 13.5 GHz to 20 GHz                                    | --                                                 | 120        | 112        | 112        | --                                           | --         | --         | --         |
| 20 GHz to 31.25 GHz                                   | --                                                 | --         | 103        | 103        | --                                           | --         | --         | --         |
| 31.25 GHz to 40 GHz                                   | --                                                 | --         | 98         | 98         | --                                           | --         | --         | --         |
| 40 GHz to 50 GHz                                      | --                                                 | --         | --         | 83         | --                                           | --         | --         | --         |

1 The direct receiver access input extended dynamic range is calculated as the difference between the direct receiver access input noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its compression or damage level. When the analyzer is in segment sweep mode, it can have predefined frequency segments which will output a higher power level when the extended dynamic range is required (i.e. devices with high insertion loss), and reduced power when receiver compression or damage may occur (i.e. devices with low insertion loss). The extended range is only available in one-path transmission measurements.

2 May be degraded by 10 dB at particular frequencies (multiples of 5 MHz) below 500 MHz due to spurious receiver residuals. Methods are available to regain the full dynamic range.

Corrected System Performance with 3.5mm Connectors (Tables 3 - 8)

Corrected System Performance with 2.4mm Connectors (Tables 9 - 12)

Corrected System Performance with Type-N Connectors (Tables 13 - 14)

**Table 15. Uncorrected System Performance**

| Description          | Specifications                         |                        |                        |                        | Typical                                |                        |                        |                        |
|----------------------|----------------------------------------|------------------------|------------------------|------------------------|----------------------------------------|------------------------|------------------------|------------------------|
|                      | Options<br>020,<br>025,<br>120,<br>125 | Options<br>220,<br>225 | Options<br>420,<br>425 | Options<br>520,<br>525 | Options<br>020,<br>025,<br>120,<br>125 | Options<br>220,<br>225 | Options<br>420,<br>425 | Options<br>520,<br>525 |
| <b>Directivity</b>   |                                        |                        |                        |                        |                                        |                        |                        |                        |
| 300 kHz to 10 MHz    | 16 dB                                  | --                     | --                     | --                     | --                                     | 23 dB                  | --                     |                        |
| 10 MHz to 45 MHz     | 28 dB                                  | --                     | --                     | --                     | --                                     |                        | 20 dB                  | 20 dB                  |
| 45 MHz to 500 MHz    | 28 dB                                  | 24 dB                  | 23 dB                  | 23 dB                  | --                                     | --                     | --                     | --                     |
| 500 MHz to 1 GHz     | 28 dB                                  | 27 dB                  | 23 dB                  | 23 dB                  | --                                     | --                     | --                     | --                     |
| 1 GHz to 2 GHz       | 25 dB                                  | 27 dB                  | 23 dB                  | 23 dB                  | --                                     | --                     | --                     | --                     |
| 2 GHz to 3 GHz       | 25 dB                                  | 21 dB                  | 21 dB                  | 21 dB                  | --                                     | --                     | --                     | --                     |
| 3 GHz to 5 GHz       | 20 dB                                  | 21 dB                  | 21 dB                  | 21 dB                  | --                                     | --                     | --                     | --                     |
| 5 GHz to 8 GHz       | 17 dB                                  | 21 dB                  | 21 dB                  | 21 dB                  | --                                     | --                     | --                     | --                     |
| 8 GHz to 11.5 GHz    | 17 dB                                  | 16 dB                  | 16 dB                  | 16 dB                  | --                                     | --                     | --                     | --                     |
| 11.5 GHz to 13.5 GHz | 15 dB                                  | 16 dB                  | 16 dB                  | 16 dB                  | --                                     | --                     | --                     | --                     |
| 13.5 GHz to 20 GHz   | --                                     | 16 dB                  | 16 dB                  | 16 dB                  | --                                     | --                     | --                     | --                     |
| 20 GHz to 40 GHz     | --                                     | --                     | 15 dB                  | 15 dB                  | --                                     | --                     | --                     | --                     |
| 45 GHz to 50 GHz     | --                                     | --                     | --                     | 13 dB                  | --                                     | --                     | --                     | --                     |
| <b>Source Match</b>  |                                        |                        |                        |                        |                                        |                        |                        |                        |
| 300 kHz to 10 MHz    | 18 dB                                  | --                     | --                     | --                     | --                                     | --                     | --                     | --                     |

|                      |       |       |       |       |    |       |       |       |
|----------------------|-------|-------|-------|-------|----|-------|-------|-------|
| 10 MHz to 45 MHz     | 25 dB | --    | --    | --    | -  | 12 dB | 11 dB | 11 dB |
| 45 MHz to 500 MHz    | 25 dB | 20 dB | 17 dB | 17 dB | -- | --    | --    | --    |
| 500 MHz to 2 GHz     | 21 dB | 17 dB | 17 dB | 17 dB | -- | --    | --    | --    |
| 2 GHz to 3 GHz       | 19 dB | 12 dB | 12 dB | 12 dB | -- | --    | --    |       |
| 3 GHz to 8 GHz       | 12 dB | 12 dB | 12 dB | 12 dB | -- | --    | --    | --    |
| 8 GHz to 9 GHz       | 12 dB | 11 dB | 11 dB | 11 dB | -- | --    | --    |       |
| 9 GHz to 12.5 GHz    | 10 dB | 11 dB | 11 dB | 11 dB | -- | --    | --    | --    |
| 12.5 GHz to 13.5 GHz | 8 dB  | 10 dB | 11 dB | 11 dB | -- | --    | --    | --    |
| 13.5 GHz to 20 GHz   | --    | 10 dB | 11 dB | 11 dB | -- | --    | --    | --    |
| 20 GHz to 40 GHz     | --    | --    | 7 dB  | 7 dB  | -- | --    | --    | --    |
| 40 GHz to 50 GHz     | --    | --    | --    | 6 dB  | -- | --    | --    | --    |

**Table 15.** Uncorrected System Performance (Continued)

| Description       | Specifications                   |                     |                     |                     | Typical                          |                     |                     |                     |
|-------------------|----------------------------------|---------------------|---------------------|---------------------|----------------------------------|---------------------|---------------------|---------------------|
|                   | Options<br>020, 025,<br>120, 125 | Options<br>220, 225 | Options<br>420, 425 | Options<br>520, 525 | Options<br>020, 025,<br>120, 125 | Options<br>220, 225 | Options<br>420, 425 | Options<br>520, 525 |
| <b>Load Match</b> |                                  |                     |                     |                     |                                  |                     |                     |                     |
| 300 kHz to 10 MHz | 17 dB                            | --                  | --                  | --                  | --                               | --                  | --                  | --                  |
| 10 MHz to 45 MHz  | 22 dB                            | --                  | --                  | --                  | --                               | 15 dB               | 13 dB               | 13 dB               |

|                      |       |       |       |        |    |    |    |    |
|----------------------|-------|-------|-------|--------|----|----|----|----|
| 45 MHz to 500 MHz    | 22 dB | 22 dB | 18 dB | 18 dB  | -- | -- | -- | -- |
| 500 MHz to 2 GHz     | 17 dB | 20 dB | 18 dB | 18 dB  | -- | -- | -- | -- |
| 2 GHz to 3 GHz       | 14 dB | 12 dB | 14 dB | 14 dB  | -- | -- | -- | -- |
| 3 GHz to 8 GHz       | 10 dB | 12 dB | 14 dB | 14 dB  | -- | -- | -- | -- |
| 8 GHz to 9 GHz       | 9 dB  | 10 dB | 12 dB | 12 dB  | -- | -- | -- | -- |
| 9 GHz to 12.5 GHz    | 9 dB  | 10 dB | 12 dB | 12 dB  | -- | -- | -- | -- |
| 12.5 GHz to 13.5 GHz | 7 dB  | 9 dB  | 9 dB  | 9.5 dB | -- | -- | -- | -- |
| 13.5 GHz to 20 GHz   | --    | 9 dB  | 9 dB  | 9.5 dB | -- | -- | -- | -- |
| 20 GHz to 40 GHz     | --    | --    | 8 dB  | 8.5 dB | -- | -- | -- | -- |
| 40 GHz to 50 GHz     | --    | --    | --    | 5 dB   | -- | -- | -- | -- |

**Table 15.** Uncorrected System Performance (Continued)

| Description                  | Specifications                   |                     |                     |                     | Typical                          |                     |                     |                     |
|------------------------------|----------------------------------|---------------------|---------------------|---------------------|----------------------------------|---------------------|---------------------|---------------------|
|                              | Options<br>020, 025,<br>120, 125 | Options<br>220, 225 | Options<br>420, 425 | Options<br>520, 525 | Options<br>020, 025,<br>120, 125 | Options<br>220, 225 | Options<br>420, 425 | Options<br>520, 525 |
| <b>Crosstalk<sup>1</sup></b> |                                  |                     |                     |                     |                                  |                     |                     |                     |
| 300 kHz to 10 MHz            | --                               | --                  | --                  | --                  | 80 dB                            | --                  | --                  | --                  |
| 10 MHz to 45 MHz             | --                               | --                  | --                  | --                  | 115 dB                           | 88 dB               | 88 dB               | 88 dB               |
| 45 MHz to 500 MHz            | --                               | --                  | --                  | --                  | 122 dB                           | 95 dB               | 94 dB               | 94 dB               |

|                      |    |    |    |    |        |        |        |        |
|----------------------|----|----|----|----|--------|--------|--------|--------|
| 500 MHz to 2 GHz     | -- | -- | -- | -- | 122 dB | 96 dB  | 95 dB  | 95 dB  |
| 2 GHz to 8 GHz       | -- | -- | -- | -- | 122 dB | 110 dB | 108 dB | 108 dB |
| 8 GHz to 10.5 GHz    | -- | -- | -- | -- | 120 dB | 116 dB | 113 dB | 113 dB |
| 10.5 GHz to 12.5 GHz | -- | -- | -- | -- | 115 dB | 116 dB | 113 dB | 113 dB |
| 12.5 GHz to 13.5 GHz | -- | -- | -- | -- | 109 dB | 115 dB | 112 dB | 112 dB |
| 13.5 GHz to 20 GHz   | -- | -- | -- | -- | --     | 115 dB | 112 dB | 112 dB |
| 20 GHz to 40 GHz     | -- | -- | -- | -- | --     | --     | 97 dB  | 97 dB  |
| 40 GHz to 50 GHz     | -- | -- | -- | -- | --     | --     | --     | 89 dB  |

1 Measurement conditions: normalized to a thru, measured with two shorts, 10 Hz IF bandwidth, averaging factor of 8, alternate mode, source power set to the specified maximum power output or the minimum receiver input power specified by the 0.1 dB compression power.

**Table 16.** Test Port Output<sup>1</sup>

| Description                                                     | Specifications         |                     |                        |                     |                        | Typicals                            |                        |                        |                     |
|-----------------------------------------------------------------|------------------------|---------------------|------------------------|---------------------|------------------------|-------------------------------------|------------------------|------------------------|---------------------|
|                                                                 | Options<br>020,<br>025 | Options<br>120, 125 | Options<br>220,<br>225 | Options<br>420, 425 | Options<br>520,<br>525 | Options<br>020,<br>025,<br>120, 125 | Options<br>220,<br>225 | Options<br>420,<br>425 | Options<br>520, 525 |
| <b>Frequency Range</b>                                          |                        |                     |                        |                     |                        |                                     |                        |                        |                     |
| N5230A                                                          | 300kHz to 6 GHz        | 300kHz to 13.5 GHz  | 10 MHz to 20 GHz       | 10 MHz to 40 GHz    | 10 MHz to 50 GHz       | --                                  |                        |                        |                     |
| <b>Nominal Power</b>                                            |                        |                     |                        |                     |                        |                                     |                        |                        |                     |
| Preset power; attenuator switch point 10 dB below nominal power |                        |                     |                        |                     |                        |                                     |                        |                        |                     |
|                                                                 | 0 dBm                  | 0 dBm               | -5 dBm                 | -10 dBm             | -15 dBm                | --                                  |                        |                        |                     |
| <b>Frequency Resolution</b>                                     |                        |                     |                        |                     |                        |                                     |                        |                        |                     |
|                                                                 | 1 Hz                   |                     |                        |                     |                        | --                                  |                        |                        |                     |
| <b>CW Accuracy</b>                                              |                        |                     |                        |                     |                        |                                     |                        |                        |                     |

|                            |          |                                                     |
|----------------------------|----------|-----------------------------------------------------|
|                            | +/-1 ppm | --                                                  |
| <b>Frequency Stability</b> |          |                                                     |
|                            | --       | +/-0.05 ppm. -10° to 70° C<br>+/-0.1 ppm/yr maximum |

**Table 16.** Test Port Output<sup>1</sup> (Continued)

| Description                             | Specifications     |           |           |           |           | Typical            |           |                    |
|-----------------------------------------|--------------------|-----------|-----------|-----------|-----------|--------------------|-----------|--------------------|
|                                         | Options            | Options   | Options   | Option    | Option    | Options            | Option    | Option             |
|                                         | 020, 025, 120, 125 | 220, 225  | 420, 425  | 520       | 525       | 020, 025, 120, 125 | 220, 225  | 420, 425, 520, 525 |
| <b>Power Level Accuracy</b>             |                    |           |           |           |           |                    |           |                    |
| Variation from nominal power in range 0 |                    |           |           |           |           |                    |           |                    |
| 300 kHz to 10 MHz                       | +/-1.0 dB          | --        | --        | --        | --        | --                 | --        | --                 |
| 10 MHz to 45 MHz                        | +/-1.0 dB          | --        | --        | --        | --        | --                 | +/-0.5 dB | +/-0.5 dB          |
| 45 MHz to 6 GHz                         | +/-1.0 dB          | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | --                 | --        | --                 |
| 6 GHz to 8 GHz                          | +/-1.5 dB          | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | --                 | --        | --                 |
| 8 GHz to 9 GHz                          | +/-1.5 dB          | +/-1.0 dB | +/-1.5 dB | +/-1.5 dB | +/-1.5 dB | --                 | --        | --                 |
| 9 GHz to 10.5 GHz                       | +/-1.5 dB          | +/-1.0 dB | +/-1.5 dB | +/-1.5 dB | +/-1.5 dB | --                 | --        | --                 |
| 10.5 GHz to 13.5 GHz                    | +/-2.0 dB          | +/-1.0 dB | +/-1.5 dB | +/-1.5 dB | +/-1.5 dB | --                 | --        | --                 |
| 13.5 to 20 GHz                          | --                 | +/-1.0 dB | +/-1.5 dB | +/-1.5 dB | +/-1.5 dB | --                 | --        | --                 |



|                  |    |    |           |           |           |    |    |    |
|------------------|----|----|-----------|-----------|-----------|----|----|----|
| 20 GHz to 40 GHz | -- | -- | +/-2.5 dB | +/-2.5 dB | +/-2.5 dB | -- | -- | -- |
| 40 GHz to 50 GHz | -- | -- | --        | +/-3.5 dB | +/-3.5 dB | -- | -- | -- |

**Table 16.** Test Port Output<sup>1</sup> (Continued)

|                           | Specifications   |                  |                  |            |            |            |            | Typical              |
|---------------------------|------------------|------------------|------------------|------------|------------|------------|------------|----------------------|
|                           | Options 020, 120 | Options 025, 125 | Options 220, 225 | Option 420 | Option 425 | Option 520 | Option 525 | Options as Indicated |
| <b>Max Levelled Power</b> |                  |                  |                  |            |            |            |            |                      |
| 300 kHz to 10 MHz         | 10 dBm           | 9 dBm            | --               | --         | --         | --         | --         | --                   |
| 10 MHz to 45 MHz          | 10 dBm           | 9 dBm            | --               | --         | --         | --         | --         | --                   |
| 45 MHz to 6 GHz           | 10 dBm           | 9 dBm            | 5 dBm            | 0 dBm      | 0 dBm      | 0 dBm      | 0 dBm      | --                   |
| 6 GHz to 9 GHz            | 8 dBm            | 8 dBm            | 5 dBm            | 0 dBm      | 0 dBm      | 0 dBm      | 0 dBm      | --                   |
| 9 GHz to 12.5 GHz         | 4 dBm            | 4 dBm            | 5 dBm            | 0 dBm      | 0 dBm      | 0 dBm      | 0 dBm      | --                   |
| 12.5 GHz to 13.5 GHz      | 2 dBm            | 1 dBm            | 3 dBm            | 0 dBm      | 0 dBm      | 0 dBm      | 0 dBm      | --                   |
| 13.5 GHz to 20 GHz        | --               | --               | 3 dBm            | 0 dBm      | 0 dBm      | 0 dBm      | 0 dBm      | --                   |
| 20 GHz to 40 GHz          | --               | --               | --               | -5 dBm     | -8 dBm     | -5 dBm     | -8 dBm     | --                   |
| 40 GHz to 50 GHz          | --               | --               | --               | --         | --         | -11 dBm    | -15 dBm    | --                   |

**Power Level Linearity<sup>2</sup>**

Test reference is at the nominal power level

|                                            |           |           |           |           |           |           |           |                                                                             |
|--------------------------------------------|-----------|-----------|-----------|-----------|-----------|-----------|-----------|-----------------------------------------------------------------------------|
| 300 kHz to 1 MHz                           | +/-4.5 dB | +/-4.5 dB | --        | --        | --        | --        | --        | +/-2.0 dB<br>(Opt 020, 025, 120, 125)                                       |
| 1 MHz to 10 MHz                            | +/-1.0 dB | +/-1.0 dB | --        | --        | --        | --        | --        | --                                                                          |
| 10 MHz to 45 MHz                           | +/-2.0 dB | +/-2.0 dB | --        | --        | --        | --        | --        | +/-0.35 dB<br>(Opt 220 & 225)<br><br>+/-0.40 dB<br>(Opt 420, 425, 520, 525) |
| 45 MHz to 1 GHz                            | +/-2.0 dB | +/-2.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | --                                                                          |
| 1 GHz to 12.5 GHz                          | +/-1.5 dB | +/-1.5 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | --                                                                          |
| 12.5 GHz to 13.5 GHz                       | +/-1.5 dB | +/-1.5 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | --                                                                          |
| 13.5 GHz to 20 GHz                         | --        | --        | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | --                                                                          |
| 20 GHz to 40 GHz                           | --        | --        | --        | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | +/-1.0 dB | --                                                                          |
| 40 GHz to 50 GHz                           | --        | --        | --        | --        | --        | +/-1.0 dB | +/-1.0 dB | --                                                                          |
| <b>Power Sweep Range (ALC)<sup>3</sup></b> |           |           |           |           |           |           |           |                                                                             |
| 300 kHz to 10 MHz                          | 37 dB     | 36 dB     | --        | --        | --        | --        | --        | --                                                                          |
| 10 MHz to 45 MHz                           | 37 dB     | 36 dB     | --        | --        | --        | --        | --        | --                                                                          |
| 45 MHz to 6 GHz                            | 37 dB     | 36 dB     | 25 dB     | 25 dB     | 25 dB     | 25 dB     | 25 dB     | --                                                                          |

|                      |       |       |       |       |       |       |       |    |
|----------------------|-------|-------|-------|-------|-------|-------|-------|----|
| 6 GHz to 9 GHz       | 35 dB | 35 dB | 25 dB | 25 dB | 25 dB | 25 dB | 25 dB | -- |
| 9 GHz to 12.5 GHz    | 31 dB | 31 dB | 25 dB | 25 dB | 25 dB | 25 dB | 25 dB | -- |
| 12.5 GHz to 13.5 GHz | 29 dB | 28 dB | 23 dB | 25 dB | 25 dB | 25 dB | 25 dB | -- |
| 13.5 GHz to 20 GHz   | --    | --    | 23 dB | 25 dB | 25 dB | 25 dB | 25 dB | -- |
| 20 GHz to 40 GHz     | --    | --    | --    | 20 dB | 17 dB | 20 dB | 17 dB | -- |
| 40 GHz to 50 GHz     | --    | --    | --    | --    | --    | 14 dB | 10 dB | -- |

**Power Resolution**

0.01 dB

**Table 16.** Test Port Output<sup>1</sup> (Continued)

| Description        | Specifications | Typical         |                 |                |                |                 |                 |
|--------------------|----------------|-----------------|-----------------|----------------|----------------|-----------------|-----------------|
|                    |                | Option 020, 120 | Option 025, 125 | Option 220     | Option 225     | Option 420, 520 | Option 425, 525 |
| <b>Power Range</b> |                |                 |                 |                |                |                 |                 |
| 300 kHz to 10 MHz  | --             | -30 to +10 dBm  | -90 to +9 dBm   | --             | --             | --              | --              |
| 10 MHz to 45 MHz   | --             | -30 to +10 dBm  | -90 to +9 dBm   | -27 to +14 dBm | -87 to +12 dBm | -27 to +9 dBm   | -87 to +8 dBm   |
| 45 MHz to 6 GHz    | --             | -30 to +10 dBm  | -90 to +9 dBm   | -27 to +14 dBm | -87 to +12 dBm | -27 to +8 dBm   | -87 to +8 dBm   |
| 6 GHz to 9 GHz     | --             | -30 to +8 dBm   | -90 to +8 dBm   | -27 to +14 dBm | -87 to +12 dBm | -27 to +8 dBm   | -87 to +8 dBm   |

|                      |    |               |               |                |                |               |               |
|----------------------|----|---------------|---------------|----------------|----------------|---------------|---------------|
| 9 GHz to 12.5 GHz    | -- | -30 to +4 dBm | -90 to +4 dBm | -27 to +14 dBm | -87 to +12 dBm | -27 to +8 dBm | -87 to +8 dBm |
| 12.5 GHz to 13.5 GHz | -- | -30 to +2 dBm | -90 to +1 dBm | -27 to +10 dBm | -87 to +7 dBm  | -27 to +5 dBm | -87 to +4 dBm |
| 13.5 GHz to 20 GHz   | -- | --            | --            | -27 to +10 dBm | -87 to +7 dBm  | -27 to +5 dBm | -87 to +4 dBm |
| 20 GHz to 40 GHz     | -- | --            | --            | --             | --             | -27 to +1 dBm | -87 to -2 dBm |
| 40 GHz to 50 GHz     | -- | --            | --            | --             | --             | -27 to -5 dBm | -87 to -9 dBm |

**Power Settings**

|                       |    |         |         |         |         |         |         |
|-----------------------|----|---------|---------|---------|---------|---------|---------|
| Minimum Power Setting | -- | -33 dBm | -93 dBm | -30 dBm | -90 dBm | -30 dBm | -90 dBm |
| Maximum Power Setting | -- | +20 dBm |         |         |         |         |         |

**Table 16.** Test Port Output<sup>1</sup> (Continued)

| Description | Specifications | Typical                    |                                      |
|-------------|----------------|----------------------------|--------------------------------------|
|             | --             | Options 020, 025, 120, 125 | Options 220, 225, 420, 425, 520, 525 |

**Phase Noise (Nominal power at test port)**

|                      | Specifications | 10 kHz Offset | 100 kHz Offset | 1 MHz Offset | 10 kHz Offset | 100 kHz Offset | 1 MHz Offset |
|----------------------|----------------|---------------|----------------|--------------|---------------|----------------|--------------|
| 300 kHz to 10 MHz    | --             | -86 dBc/Hz    | -86 dBc/Hz     | -95 dBc/Hz   | -77 dBc/Hz    | -77 dBc/Hz     | -40 dBc/Hz   |
| 10 MHz to 1.5 GHz    | --             | -86 dBc/Hz    | -91 dBc/Hz     | -95 dBc/Hz   | -77 dBc/Hz    | -77 dBc/Hz     | -89 dBc/Hz   |
| 1.5 GHz to 3.125 GHz | --             | -83 dBc/Hz    | -91 dBc/Hz     | -95 dBc/Hz   | -83 dBc/Hz    | -91 dBc/Hz     | -95 dBc/Hz   |

|                       |    |            |            |            |            |            |            |
|-----------------------|----|------------|------------|------------|------------|------------|------------|
| 3.125 GHz to 6.25 GHz | -- | -77 dBc/Hz | -85 dBc/Hz | -89 dBc/Hz | -77 dBc/Hz | -85 dBc/Hz | -89 dBc/Hz |
| 6.25 GHz to 12.5 GHz  | -- | -71 dBc/Hz | -79 dBc/Hz | -83 dBc/Hz | -71 dBc/Hz | -79 dBc/Hz | -83 dBc/Hz |
| 12.5 GHz to 13.5 GHz  | -- | -65 dBc/Hz | -73 dBc/Hz | -77 dBc/Hz | -65 dBc/Hz | -73 dBc/Hz | -77 dBc/Hz |
| 13.5 GHz to 20 GHz    | -- | --         | --         | --         | -65 dBc/Hz | -73 dBc/Hz | -77 dBc/Hz |
| 20 GHz to 40 GHz      | -- | --         | --         | --         | -59 dBc/Hz | -67 dBc/Hz | -71 dBc/Hz |
| 40 GHz to 50 GHz      | -- | --         | --         | --         | -59 dBc/Hz | -67 dBc/Hz | -71 dBc/Hz |

**Table 16.** Test Port Output<sup>1</sup> (Continued)

| Description                                            | Specifications | Typicals                                                 |
|--------------------------------------------------------|----------------|----------------------------------------------------------|
|                                                        | --             | Options 020, 025, 120, 125, 220, 225, 420, 520, 425, 525 |
| <b>Non-Harmonic Spurious (at Nominal Output Power)</b> |                |                                                          |
| 300 kHz to 10 MHz                                      | --             | -50 dBc for offset frequency > 1 kHz                     |
| 10 MHz to 13.5 GHz                                     | --             |                                                          |
| 13.5 GHz to 20 GHz                                     | --             |                                                          |
| 20 GHz to 40 GHz                                       | --             | -30 dBc for offset frequency > 1 kHz                     |
| 40 GHz to 50 GHz                                       | --             |                                                          |

**Table 16.** Test Port Output<sup>1</sup> (Continued)

| Description | Specifications | Typical |
|-------------|----------------|---------|
|-------------|----------------|---------|

|                                                       |    |                                    |                       |                    |                    |
|-------------------------------------------------------|----|------------------------------------|-----------------------|--------------------|--------------------|
|                                                       | -- | Option<br>020,<br>025,<br>120, 125 | Option<br>220,<br>225 | Option<br>420, 520 | Option<br>425, 525 |
| <b>Harmonics (2nd or 3rd) at Maximum Output Power</b> |    |                                    |                       |                    |                    |
| 300 kHz to<br>10 MHz                                  | -- | -17 dBc                            | --                    | --                 | --                 |
| 10 MHz to<br>500 MHz                                  | -- | -17 dBc                            | -22 dBc               | -15 dBc            | -15 dBc            |
| 500 MHz to<br>1 GHz                                   | -- | -17 dBc                            | -22 dBc               | -15 dBc            | -15 dBc            |
| 1 GHz to<br>13.5 GHz                                  | -- | -20 dBc                            | 22 dBc                | -20 dBc            | -20 dBc            |
| 13.5 GHz to<br>20 GHz                                 | -- | --                                 | -22 dBc               | -20 dBc            | -20 dBc            |
| 20 GHz to<br>40 GHz                                   | -- | --                                 | --                    | -22 dBc            | -22 dBc            |
| 40 GHz to<br>50 GHz                                   | -- | --                                 | --                    | --                 | -22 dBc            |

1Performance specified on Port 1 only. Port 2 performance is a characteristic.

2Power level linearity specified on Port 1 only. Port 2 performance is Typical. Test reference is at the nominal power level.

3ALC range starts at maximum leveled power and decreases in power level by the dB amount specified here.

**Table 17. Test Port Input**

| Description                              | Specification                          |                        |                        |                        | Typical                                |                        |                        |                        |
|------------------------------------------|----------------------------------------|------------------------|------------------------|------------------------|----------------------------------------|------------------------|------------------------|------------------------|
|                                          | Options<br>020,<br>025,<br>120,<br>125 | Options<br>220,<br>225 | Options<br>420,<br>425 | Options<br>520,<br>525 | Options<br>020,<br>025,<br>120,<br>125 | Options<br>220,<br>225 | Options<br>420,<br>425 | Options<br>520,<br>525 |
| <b>Test Port Noise Floor<sup>1</sup></b> |                                        |                        |                        |                        |                                        |                        |                        |                        |
| <b>10 Hz IF Bandwidth</b>                |                                        |                        |                        |                        |                                        |                        |                        |                        |
| 300 kHz to 1<br>MHz                      | <-93<br>dBm                            | --                     | --                     | --                     | <-103<br>dBm                           | --                     | --                     | --                     |
| 1 MHz to 10<br>MHz                       | <-103<br>dBm                           | --                     | --                     | --                     | <-110<br>dBm                           | --                     | --                     | --                     |

|                           |           |           |           |           |           |          |          |          |
|---------------------------|-----------|-----------|-----------|-----------|-----------|----------|----------|----------|
| 10 MHz to 45 MHz          | <-112 dBm | --        | --        | --        | <-116 dBm | <-89 dBm | <-80 dBm | <-80 dBm |
| 45 MHz to 500 MHz         | <-112 dBm | <-100 dBm | <-90 dBm  | <-90 dBm  | <-116 dBm | --       | --       | --       |
| 500 MHz to 2 GHz          | <-112 dBm | <-105 dBm | <-110 dBm | <-110 dBm | <-120 dBm | --       | --       | --       |
| 2 GHz to 4 GHz            | <-112 dBm | <-105 dBm | <-110 dBm | <-110 dBm | <-120 dBm | --       | --       | --       |
| 4 GHz to 8 GHz            | <-112 dBm | <-105 dBm | <-110 dBm | <-110 dBm | <-119 dBm | --       | --       | --       |
| 8 GHz to 10.5 GHz         | <-112 dBm | <-105 dBm | <-100 dBm | <-100 dBm | <-119 dBm | --       | --       | --       |
| 10.5 GHz to 13.5 GHz      | <-107 dBm | <-105 dBm | <-100 dBm | <-100 dBm | <-114 dBm | --       | --       | --       |
| 10.5 GHz to 13.5 GHz      | --        | <-105 dBm | <-100 dBm | <-100 dBm | --        | --       | --       | --       |
| 13.5 GHz to 20 GHz        | --        | <-105 dBm | <-100 dBm | <-100 dBm | --        | --       | --       | --       |
| 20 GHz to 31.25 GHz       | --        | --        | <-100 dBm | <-100 dBm | --        | --       | --       | --       |
| 31.25 GHz to 40 GHz       | --        | --        | <-95 dBm  | <-95 dBm  | --        | --       | --       | --       |
| 40 GHz to 50 GHz          | --        | --        | --        | <-90 dBm  | --        | --       | --       | --       |
| <b>1 KHz IF Bandwidth</b> |           |           |           |           |           |          |          |          |
| 3000 kHz to 1 MHz         | <-73 dBm  | --        | --        | --        | <-83 dBm  | --       | --       | --       |
| 1 MHz to 10 MHz           | <-83 dBm  | --        | --        | --        | <-90 dBm  | --       | --       | --       |
| 10 MHz to 45 MHz          | <-92 dBm  | --        | --        | --        | <-96 dBm  | <-69 dBm | <-60 dBm | <-60 dBm |
| 45 MHz to 500 MHz         | <-92 dBm  | <-80 dBm  | <-70 dBm  | <-70 dBm  | <-96 dBm  | --       | --       | --       |
| 500 MHz to 2 GHz          | <-92 dBm  | <-85 dBm  | <-90 dBm  | <-90 dBm  | <-100 dBm | --       | --       | --       |

|                      |          |          |          |          |           |    |    |    |
|----------------------|----------|----------|----------|----------|-----------|----|----|----|
| 2 GHz to 4 GHz       | <-92 dBm | <-85 dBm | <-90 dBm | <-90 dBm | <-100 dBm | -- | -- | -- |
| 4 GHz to 8 GHz       | <-92 dBm | <-85 dBm | <-90 dBm | <-90 dBm | <-99 dBm  | -- | -- | -- |
| 8 GHz to 10.5 GHz    | <-92 dBm | <-85 dBm | <-80 dBm | <-80 dBm | <-99 dBm  | -- | -- | -- |
| 10.5 GHz to 13.5 GHz | <-87 dBm | <-85 dBm | <-80 dBm | <-80 dBm | <-94 dBm  | -- | -- | -- |
| 13.5 GHz to 20 GHz   | --       | <-85 dBm | <-80 dBm | <-80 dBm | --        | -- | -- | -- |
| 20 GHz to 31.25 GHz  | --       | --       | <-80 dBm | <-80 dBm | --        | -- | -- | -- |
| 31.25 GHz to 40 GHz  | --       | --       | <-75 dBm | <-75 dBm | --        | -- | -- | -- |
| 40 GHz to 50 GHz     | --       | --       | --       | <-70 dBm | --        | -- | -- | -- |

**Table 17.** Test Port Input (Continued)

| Description                                                                                            | Specification    |             |             |             | Typical          |             |             |             |
|--------------------------------------------------------------------------------------------------------|------------------|-------------|-------------|-------------|------------------|-------------|-------------|-------------|
|                                                                                                        | Options 025, 125 | Options 225 | Options 425 | Options 525 | Options 025, 125 | Options 225 | Options 425 | Options 525 |
| <b>Direct Receiver Access Input Noise Floor<sup>1</sup> (Options 025, 125, 225, 425, and 525 only)</b> |                  |             |             |             |                  |             |             |             |
| <b>10 Hz IF Bandwidth</b>                                                                              |                  |             |             |             |                  |             |             |             |
| 300 kHz to 1 MHz                                                                                       | <-109 dBm        | --          | --          | --          | --               | --          | --          | --          |
| 1 MHz to 10 MHz                                                                                        | <-119 dBm        | --          | --          | --          | --               | --          | --          | --          |
| 10 MHz to 45 MHz                                                                                       | <-128 dBm        | --          | --          | --          | --               | <-120 dBm   | <-126 dBm   | <-126 dBm   |
| 45 MHz to 500 MHz                                                                                      | <-128 dBm        | <-112 dBm   | <-111 dBm   | <-111 dBm   | --               | --          | --          | --          |
| 500 MHz to 2 GHz                                                                                       | <-128 dBm        | <-117 dBm   | <-122 dBm   | <-122 dBm   | --               | --          | --          | --          |



|                           |           |           |           |           |    |           |           |           |
|---------------------------|-----------|-----------|-----------|-----------|----|-----------|-----------|-----------|
| 2 GHz to 8 GHz            | <-128 dBm | <-117 dBm | <-122 dBm | <-122 dBm | -- | --        | --        | --        |
| 8 GHz to 10.5 GHz         | <-128 dBm | <-117 dBm | <-112 dBm | <-112 dBm | -- | --        | --        | --        |
| 10.5 GHz to 13.5 GHz      | <-128 dBm | <-117 dBm | <-112 dBm | <-112 dBm | -- | --        | --        | --        |
| 13.5 GHz to 20 GHz        | <-123 dBm | <-117 dBm | <-112 dBm | <-112 dBm | -- | --        | --        | --        |
| 20 GHz to 31.25 GHz       | --        | --        | <-111 dBm | <-111 dBm | -- | --        | --        | --        |
| 31.25 GHz to 40 GHz       | --        | --        | <-106 dBm | <-106 dBm | -- | --        | --        | --        |
| 40 GHz to 50 GHz          | --        | --        | --        | <-98 dBm  | -- | --        | --        | --        |
| <b>1 KHz IF Bandwidth</b> |           |           |           |           |    |           |           |           |
| 300 kHz to 1 MHz          | <-89 dBm  | --        | --        | --        | -- | --        | --        | --        |
| 1 MHz to 10 MHz           | <-99 dBm  | --        | --        | --        | -- | --        | --        | --        |
| 10 MHz to 45 MHz          | <-108 dBm | --        | --        | --        | -- | <-100 dBm | <-106 dBm | <-106 dBm |
| 45 MHz to 500 MHz         | <-108 dBm | <-92 dBm  | <-91 dBm  | <-91 dBm  | -- | --        | --        | --        |
| 500 MHz to 2 GHz          | <-108 dBm | <-97 dBm  | <-102 dBm | <-102 dBm | -- | --        | --        | --        |
| 2 GHz to 8 GHz            | <-108 dBm | <-97 dBm  | <-102 dBm | <-102 dBm | -- | --        | --        | --        |
| 8 GHz to 10.5 GHz         | <-108 dBm | <-97 dBm  | <-92 dBm  | <-92 dBm  | -- | --        | --        | --        |
| 10.5 GHz to 13.5 GHz      | <-108 dBm | <-97 dBm  | <-92 dBm  | <-92 dBm  | -- | --        | --        | --        |
| 13.5 GHz to 20 GHz        | <-103 dBm | <-97 dBm  | <-92 dBm  | <-92 dBm  | -- | --        | --        | --        |
| 20 GHz to 31.25 GHz       | --        | --        | <-91 dBm  | <-91 dBm  | -- | --        | --        | --        |

|                     |    |    |          |          |    |    |    |    |
|---------------------|----|----|----------|----------|----|----|----|----|
| 31.25 GHz to 40 GHz | -- | -- | <-86 dBm | <-86 dBm | -- | -- | -- | -- |
| 40 GHz to 50 GHz    | -- | -- | --       | <-78 dBm | -- | -- | -- | -- |

**Table 17. Test Port Input (Continued)**

| Description                   | Specification    |                          |                  |                          |                  |                          | Typical |    |    |
|-------------------------------|------------------|--------------------------|------------------|--------------------------|------------------|--------------------------|---------|----|----|
|                               | Options 220, 225 |                          | Options 420, 520 |                          | Options 425, 525 |                          | --      | -- | -- |
| <b>Compression Level</b>      |                  |                          |                  |                          |                  |                          |         |    |    |
|                               | <b>Power</b>     | <b>Com-<br/>pression</b> | <b>Power</b>     | <b>Com-<br/>pression</b> | <b>Power</b>     | <b>Com-<br/>pression</b> | --      | -- | -- |
| 10 MHz to 45 MHz <sup>2</sup> | --               | --                       | --               | --                       | --               | --                       | --      | -- | -- |
| 45 MHz to 500 MHz             | +5 dBm           | 0.10 dB                  | +5 dBm           | 0.40 dB                  | +5 dBm           | 0.40 dB                  | --      | -- | -- |
| 500 MHz to 2 GHz              | +5 dBm           | 0.15 dB                  | +5 dBm           | 0.77 dB                  | +5 dBm           | 0.67 dB                  | --      | -- | -- |
| 2 GHz to 8 GHz                | +5 dBm           | 0.21 dB                  | +5 dBm           | 0.75 dB                  | +5 dBm           | 0.55 dB                  | --      | -- | -- |
| 8 GHz to 12.5 GHz             | +5 dBm           | 0.21 dB                  | +5 dBm           | 0.56 dB                  | +5 dBm           | 0.51 dB                  | --      | -- | -- |
| 12.5 GHz to 20 GHz            | +3 dBm           | 0.20 dB                  | +5 dBm           | 0.79 dB                  | +5 dBm           | 0.69 dB                  | --      | -- | -- |
| 20 GHz to 31.25 GHz           | --               | --                       | 0 dBm            | 0.60 dB                  | 0 dBm            | 0.50 dB                  | --      | -- | -- |
| 31.25 GHz to 40 GHz           | --               | --                       | -3 dBm           | 0.55 dB                  | -3 dBm           | 0.60 dB                  | --      | -- | -- |
| 40 GHz to 50 GHz              | --               | --                       | -3 dBm           | 0.66 dB                  | -3 dBm           | 0.71 dB                  | --      | -- | -- |

**Table 17. Test Port Input (Continued)**

| Description                          | Specification                               |                                   | Typical |    |    |
|--------------------------------------|---------------------------------------------|-----------------------------------|---------|----|----|
|                                      | <b>Options</b><br><b>020, 120, 025, 125</b> |                                   | --      |    |    |
| <b>Compression Level (continued)</b> |                                             |                                   |         |    |    |
|                                      | <b>Power</b>                                | <b>Com-<br/>pression</b>          | --      | -- | -- |
| 300 kHz to 10 MHz                    | +8 dBm                                      | 1.0 dB<br>(0.1 dB at +5 dBm typ.) | --      | -- | -- |
| 10 MHz to 50 MHz                     | +8 dBm                                      | 0.35 dB                           | --      | -- | -- |
| 50 MHz to 1GHz                       | +8 dBm                                      | 0.35 dB                           | --      | -- | -- |
| 1 GHz to 6 GHz                       | +8 dBm                                      | 0.25 dB                           | --      | -- | -- |
| 6 GHz to 8 GHz                       | +8 dBm                                      | 0.25 dB                           | --      | -- | -- |
| 8 GHz to 12.5 GHz                    | +8 dBm                                      | 0.30 dB                           | --      | -- | -- |
| 12.5 GHz to 13.5 GHz                 | +8 dBm                                      | 0.40 dB                           | --      | -- | -- |

**Table 17. Test Port Input (Continued)**

| Description                           | Specification |    | Typical                                     |                    |
|---------------------------------------|---------------|----|---------------------------------------------|--------------------|
|                                       | --            |    | <b>Options</b><br><b>020, 120, 025, 125</b> |                    |
| <b>Test Port Compression - 0.1 dB</b> |               |    |                                             |                    |
|                                       | --            | -- | <b>Power</b>                                | <b>Compression</b> |
| 300 kHz to 10 MHz                     | --            | -- | +5 dBm                                      | 0.1 dB             |
| 10 MHz to 1 GHz                       | --            | -- | +9 dBm                                      | 0.1 dB             |
| 1 GHz to 12.5 GHz                     | --            | -- | +10 dBm                                     | 0.1 dB             |
| 12.5 GHz to 13.5 GHz                  | --            | -- | +9 dBm                                      | 0.1 dB             |

**Table 17. Test Port Input (Continued)**

| Description                                       | Specification                     |                                   |                                   | Typical                           |                                   |                                   |
|---------------------------------------------------|-----------------------------------|-----------------------------------|-----------------------------------|-----------------------------------|-----------------------------------|-----------------------------------|
|                                                   | <b>Options</b><br><b>220, 225</b> | <b>Options</b><br><b>420, 520</b> | <b>Options</b><br><b>425, 525</b> | <b>Options</b><br><b>220, 225</b> | <b>Options</b><br><b>420, 520</b> | <b>Options</b><br><b>425, 525</b> |
| <b>Test Port Compression - 0.1 dB (continued)</b> |                                   |                                   |                                   |                                   |                                   |                                   |
| 300 kHz to 10 MHz                                 | --                                | --                                | --                                | --                                | --                                | --                                |
| 10 MHz to 45 MHz <sup>2</sup>                     | --                                | --                                | --                                | negligible                        | negligible                        | negligible                        |
| 45 MHz to 500 MHz                                 | --                                | --                                | --                                | +10 dBm                           | 0.0 dBm                           | +1.0 dBm                          |
| 500 MHz to 2 GHz                                  | --                                | --                                | --                                | +9 dBm                            | 0.0 dBm                           | +1.0 dBm                          |
| 2 GHz to 12.5 GHz                                 | --                                | --                                | --                                | +6 dBm                            | 0.0 dBm                           | +1.5 dBm                          |

|                                                                      |              |              |              |              |              |              |
|----------------------------------------------------------------------|--------------|--------------|--------------|--------------|--------------|--------------|
| 12.5 GHz to 13.5 GHz                                                 | --           | --           | --           | +6 dBm       | -1.0 dBm     | 0.0 dBm      |
| 13.5 GHz to 20 GHz                                                   | --           | --           | --           | +6 dBm       | -1.0 dBm     | 0.0 dBm      |
| 20 GHz to 31.25 GHz                                                  | --           | --           | --           | --           | -5.5 dBm     | -3.0 dBm     |
| 31.25 GHz to 40 GHz                                                  | --           | --           | --           | --           | -8.5 dBm     | -7.5 dBm     |
| 40 GHz to 50 GHz                                                     | --           | --           | --           | --           | -11.5 dBm    | -10.0 dBm    |
| <b>Trace Noise Magnitude<sup>3</sup></b>                             |              |              |              |              |              |              |
| 1 kHz IF bandwidth, ratioed measurement, nominal power at test port. |              |              |              |              |              |              |
| 300 kHz to 10 MHz                                                    | --           | --           | --           | --           | --           | --           |
| 10 MHz to 45 MHz                                                     | --           | --           | --           | 0.004 dB rms | 0.015 dB rms | 0.015 dB rms |
| 45 MHz to 500 MHz                                                    | 0.004 dB rms | 0.010 dB rms | 0.010 dB rms | --           | --           | --           |
| 500 MHz to 2 GHz                                                     | 0.004 dB rms | 0.006 dB rms | 0.006 dB rms | --           | --           | --           |
| 2 GHz to 10.5 GHz                                                    | 0.004 dB rms | 0.006 dB rms | 0.006 dB rms | --           | --           | --           |
| 10.5 GHz to 13.5 GHz                                                 | 0.006 dB rms | 0.010 dB rms | 0.010 dB rms | --           | --           | --           |
| 13.5 GHz to 20 GHz                                                   | 0.006 dB rms | 0.010 dB rms | 0.010 dB rms | --           | --           | --           |
| 20 GHz to 31.25 GHz                                                  | --           | 0.010 dB rms | 0.010 dB rms | --           | --           | --           |
| 31.25 GHz to 40 GHz                                                  | --           | 0.020 dB rms | 0.020 dB rms | --           | --           | --           |
| 40 GHz to 50 GHz                                                     | --           | --           | 0.020 dB rms | --           | --           | --           |

**Table 17. Test Port Input (Continued)**

| Description                                                                  | Specification              |                     |                     | Typical                    |                     |                     |
|------------------------------------------------------------------------------|----------------------------|---------------------|---------------------|----------------------------|---------------------|---------------------|
|                                                                              | Options 020, 120, 025, 125 |                     |                     | Options 020, 120, 025, 125 |                     |                     |
| <b>Trace Noise Magnitude<sup>3</sup> (continued)</b>                         |                            |                     |                     |                            |                     |                     |
| <b>100 kHz IF bandwidth, ratioed measurement, nominal power at test port</b> |                            |                     |                     |                            |                     |                     |
| 300 kHz to 10 MHz                                                            | 12 mdB                     |                     |                     | --                         |                     |                     |
| 10 MHz to 6 GHz                                                              | 4 mdB                      |                     |                     | --                         |                     |                     |
| 6 GHz to 10.5 GHz                                                            | 4 mdB                      |                     |                     | --                         |                     |                     |
| 10.5 GHz to 13.5 GHz                                                         | 8 mdB                      |                     |                     | --                         |                     |                     |
| <b>600 kHz IF bandwidth, ratioed measurement, nominal power at test port</b> |                            |                     |                     |                            |                     |                     |
| 300 kHz to 10 MHz                                                            | --                         |                     |                     | 20 mdB                     |                     |                     |
| 10 MHz to 6 GHz                                                              | --                         |                     |                     | 8 mdB                      |                     |                     |
| 6 GHz to 10.5 GHz                                                            | --                         |                     |                     | 8 mdB                      |                     |                     |
| 10.5 GHz to 13.5 GHz                                                         | --                         |                     |                     | 10 mdB                     |                     |                     |
| <b>Table 17. Test Port Input (Continued)</b>                                 |                            |                     |                     |                            |                     |                     |
| Description                                                                  | Specification              |                     |                     | Typical                    |                     |                     |
|                                                                              | Options<br>220, 225        | Options<br>420, 520 | Options<br>425, 525 | Options<br>220, 225        | Options<br>420, 520 | Options<br>425, 525 |
| <b>Trace Noise Phase<sup>3</sup></b>                                         |                            |                     |                     |                            |                     |                     |
| 1 kHz IF bandwidth, ratioed measurement, nominal power at test port.         |                            |                     |                     |                            |                     |                     |
| 300 kHz to 10 MHz                                                            |                            |                     |                     |                            |                     |                     |
| 10 MHz to 45 MHz                                                             | --                         | --                  | --                  | 0.025° rms                 | 0.100° rms          | 0.100° rms          |

|                      |            |            |            |    |    |    |
|----------------------|------------|------------|------------|----|----|----|
| 45 MHz to 500 MHz    | 0.060° rms | 0.100° rms | 0.100° rms | -- | -- | -- |
| 500 MHz to 2 GHz     | 0.060° rms | 0.060° rms | 0.060° rms | -- | -- | -- |
| 2 GHz to 10.5 GHz    | 0.060° rms | 0.060° rms | 0.060° rms | -- | -- | -- |
| 10.5 GHz to 13.5 GHz | 0.060° rms | 0.100° rms | 0.100° rms |    |    |    |
| 13.5 GHz to 20 GHz   | 0.060° rms | 0.100° rms | 0.100° rms | -- | -- | -- |
| 20 GHz to 31.25 GHz  | --         | 0.100° rms | 0.100° rms | -- | -- | -- |
| 31.25 GHz to 40 GHz  | --         | 0.200° rms | 0.200° rms | -- | -- | -- |
| 40 GHz to 50 GHz     | --         | --         | 0.200° rms | -- | -- | -- |

**Table 17.** Test Port Input (Continued)

| Description                                                                  | Specification                     | Technical                         |
|------------------------------------------------------------------------------|-----------------------------------|-----------------------------------|
|                                                                              | <b>Options 020, 120, 025, 125</b> | <b>Options 020, 120, 025, 125</b> |
| <b>Trace Noise Phase<sup>3</sup> (continued)</b>                             |                                   |                                   |
| <b>100 kHz IF bandwidth, ratioed measurement, nominal power at test port</b> |                                   |                                   |
| 300 kHz to 10 MHz                                                            | 80 mdeg                           | --                                |
| 10 MHz to 6 GHz                                                              | 30 mdeg                           | --                                |
| 6 GHz to 10.5 GHz                                                            | 30 mdeg                           | --                                |
| 10.5 GHz to 13.5 GHz                                                         | 60 mdeg                           | --                                |
| <b>600 kHz IF bandwidth, ratioed measurement, nominal power at test port</b> |                                   |                                   |
| 300 kHz to 10 MHz                                                            | --                                | 100 mdeg                          |

|                      |    |         |
|----------------------|----|---------|
| 10 MHz to 6 GHz      | -- | 60 mdeg |
| 6 GHz to 10.5 GHz    | -- | 60 mdeg |
| 10.5 GHz to 13.5 GHz | -- | 80 mdeg |

**Table 17. Test Port Input (Continued)**

| Description                      | Specification                                            | Typical |
|----------------------------------|----------------------------------------------------------|---------|
|                                  | Options 020, 025, 120, 125, 220, 225, 420, 425, 520, 525 | --      |
| <b>Reference Level Magnitude</b> |                                                          |         |
| Range                            | +/-200 dB                                                |         |
| Resolution                       | 0.001dB                                                  |         |
| <b>Reference Level Phase</b>     |                                                          |         |
| Range                            | +/-500°                                                  |         |
| Resolution                       | 0.01°                                                    |         |

**Table 17. Test Port Input (Continued)**

| Description                            | Specification |    |    |    | Typical                   |                 |                            |
|----------------------------------------|---------------|----|----|----|---------------------------|-----------------|----------------------------|
|                                        | --            | -- | -- | -- | Option 020, 025, 120, 125 | Option 220, 225 | Options 420, 425, 520, 525 |
| <b>Stability Magnitude<sup>4</sup></b> |               |    |    |    |                           |                 |                            |
| 300 kHz to 10 MHz                      | --            | -- | -- | -- | +/-0.015 dB/°C            | --              | --                         |
| 10 MHz to 45 MHz                       | --            | -- | -- | -- | +/-0.010 dB/°C            | +/-0.015 dB/°C  | +/-0.015 dB/°C             |
| 45 MHz to 500 MHz                      | --            | -- | -- | -- | +/-0.010 dB/°C            | +/-0.010 dB/°C  | +/-0.010 dB/°C             |



|                                    |    |    |    |    |                |                |                |
|------------------------------------|----|----|----|----|----------------|----------------|----------------|
| 500 MHz to 2 GHz                   | -- | -- | -- | -- | +/-0.010 dB/°C | +/-0.010 dB/°C | +/-0.010 dB/°C |
| 2 GHz to 4 GHz                     | -- | -- | -- | -- | +/-0.015 dB/°C | +/-0.020 dB/°C | +/-0.010 dB/°C |
| 4 GHz to 8 GHz                     | -- | -- | -- | -- | +/-0.020 dB/°C | +/-0.020 dB/°C | +/-0.010 dB/°C |
| 4 GHz to 13.5 GHz                  | -- | -- | -- | -- | +/-0.020 dB/°C | +/-0.030 dB/°C | +/-0.015 dB/°C |
| 13.5 GHz to 20 GHz                 | -- | -- | -- | -- | --             | +/-0.030 dB/°C | +/-0.015 dB/°C |
| 20 GHz to 40 GHz                   | -- | -- | -- | -- | --             | --             | +/-0.040 dB/°C |
| 40 GHz to 50 GHz                   | -- | -- | -- | -- | --             | --             | +/-0.060 dB/°C |
| <b>Stability Phase<sup>4</sup></b> |    |    |    |    |                |                |                |
| 300 kHz to 10 MHz                  | -- | -- | -- | -- | +/-0.30°/°C    | --             | --             |
| 10 MHz to 45 MHz                   | -- | -- | -- | -- | +/-0.025°/°C   | +/-0.25°/°C    | +/-0.25°/°C    |
| 45 MHz to 500 MHz                  | -- | -- | -- | -- | +/-0.035°/°C   | +/-0.20°/°C    | +/-0.22°/°C    |
| 500 MHz to 2 GHz                   | -- | -- | -- | -- | +/-0.050°/°C   | +/-0.15°/°C    | +/-0.22°/°C    |
| 2 GHz to 4 GHz                     | -- | -- | -- | -- | +/-0.10°/°C    | +/-0.15°/°C    | +/-0.10°/°C    |
| 4 GHz to 8 GHz                     | -- | -- | -- | -- | +/-0.15°/°C    | +/-0.15°/°C    | +/-0.10°/°C    |
| 8 GHz to 13.5 GHz                  | -- | -- | -- | -- | +/-0.30°/°C    | +/-0.45°/°C    | +/-0.15°/°C    |
| 13.5 GHz to 20 GHz                 | -- | -- | -- | -- | --             | +/-0.45°/°C    | +/-0.15°/°C    |
| 20 GHz to 40 GHz                   | -- | -- | -- | -- | --             | --             | +/-0.40°/°C    |
| 40 GHz to 50 GHz                   | -- | -- | -- | -- | --             | --             | +/-0.40°/°C    |

**Table 17. Test Port Input (Continued)**

| Description               | Specifications | Typical               |                       |                       |                       |
|---------------------------|----------------|-----------------------|-----------------------|-----------------------|-----------------------|
|                           |                | Options 020, 120      | Option 220, 420, 520  | Options 025, 125      | Options 225, 425, 525 |
|                           | --             |                       |                       |                       |                       |
| <b>Damage Input Level</b> |                |                       |                       |                       |                       |
| Test Port 1 and 2         | --             | +27 dBm or +/- 16 VDC | +30 dBm or +/- 40 VDC | +27 dBm or +/- 16 VDC | +27 dBm or +/- 16 VDC |
| R1, R2 in                 | --             | --                    | --                    | +15 dBm or +/- 16 VDC | +15 dBm or +/- 7 VDC  |
| A, B in                   | --             | --                    | --                    | +15 dBm or +/- 16 VDC | +15 dBm or +/- 7 VDC  |
| Coupler Thru              | --             | --                    | --                    | +27 dBm or +/- 16 VDC | +30 dBm or +/- 40 VDC |
| Coupler Arm               | --             | --                    | --                    | +15 dBm or +/- 0 VDC  | +30 dBm or +/- 7 VDC  |

1Total average (rms) noise power calculated as the mean value of a linear magnitude trace expressed in dBm.

2Coupler roll-off will reduce compression to a negligible level below 45 MHz.

31 kHz IF BW, ratioed measurement, nominal power at the test port.

4Stability is defined as a ratio measurement made at the test port.


**Table 18. Dynamic Accuracy (Specification<sup>a</sup>)**

Accuracy of the test port input power reading relative to the reference input power level.


**Options 020, 025, 120, 125**

**Dynamic Accuracy, 300 kHz - 1 MHz, Option 020, 025, 120, or 125**

**Magnitude**

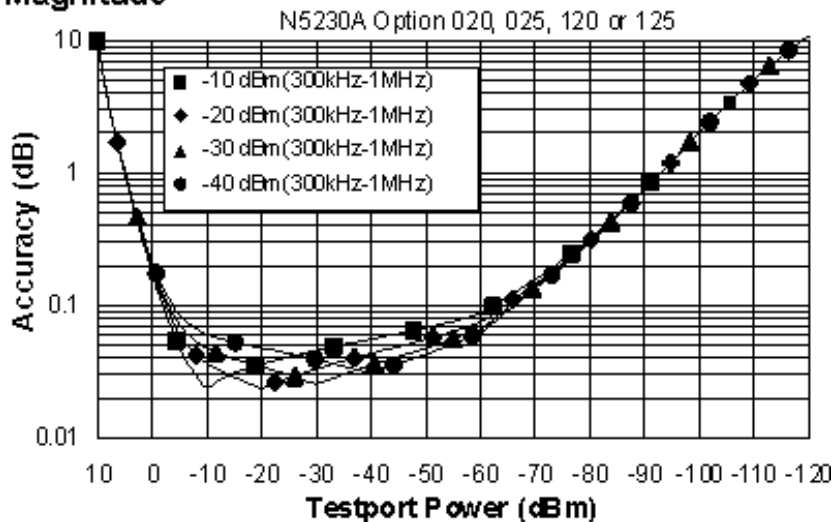


### Phase

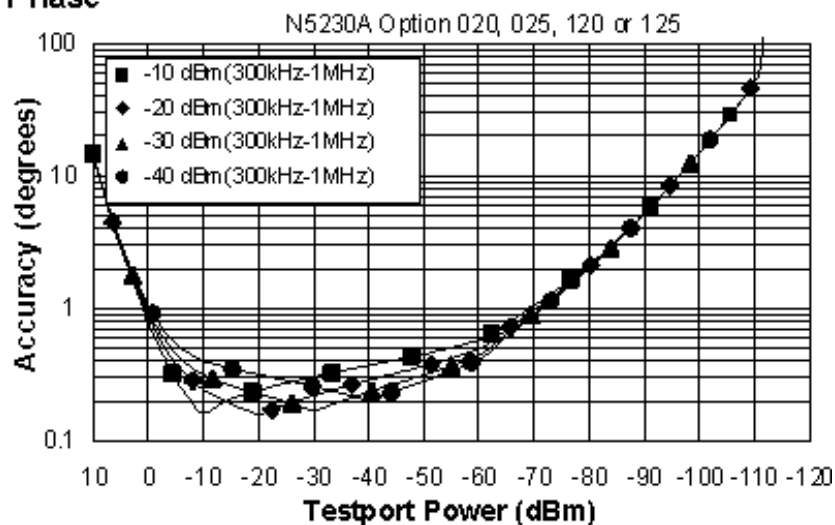


### Dynamic Accuracy, 1 MHz- 10 MHz, Option 020, 025, 120, or 125


### Magnitude

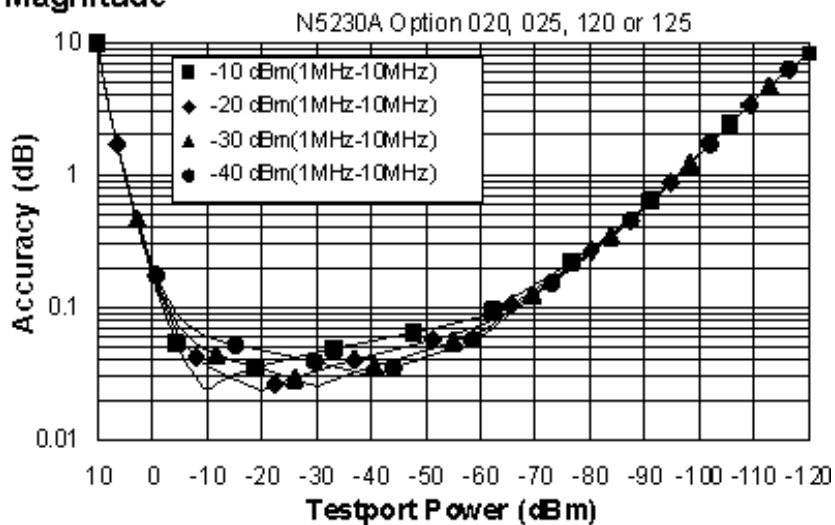


### Phase

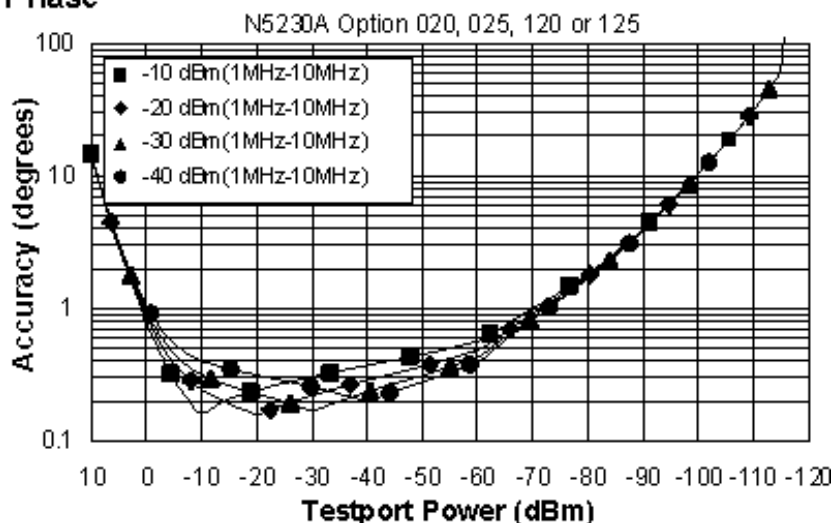


**Magnitude**

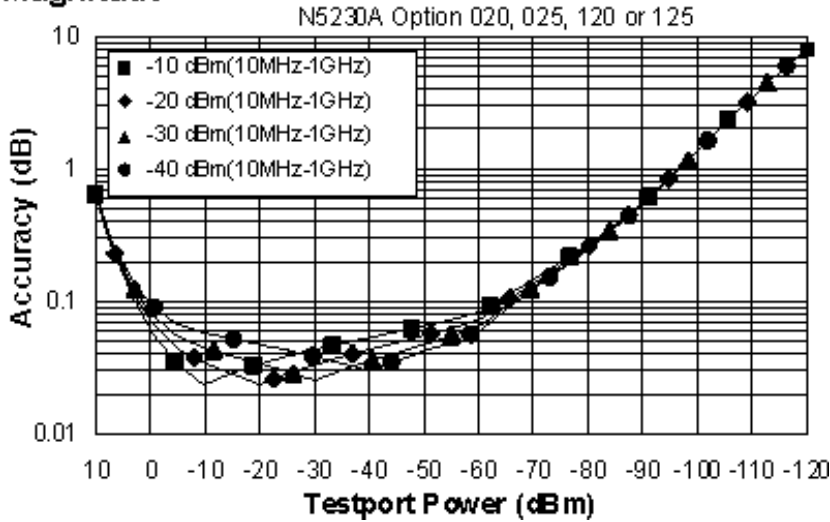


**Phase**

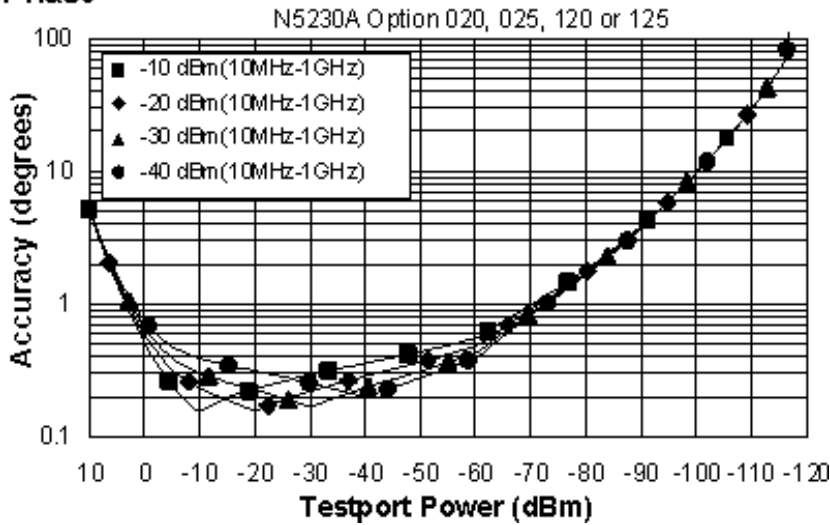

**Magnitude**

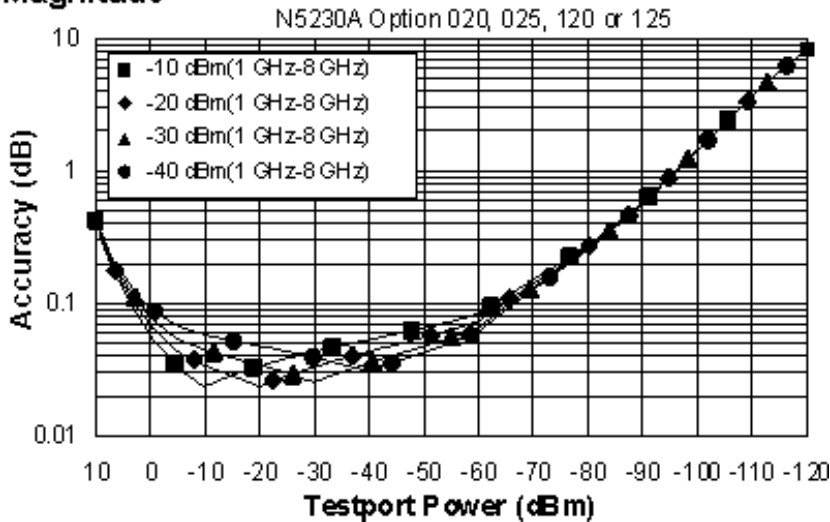


## Phase

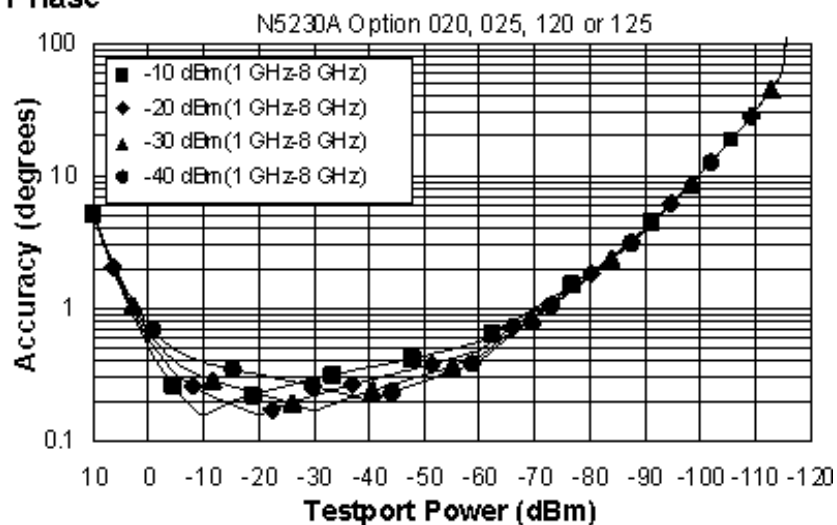


## Dynamic Accuracy, 8 - 10.5 GHz, Option 120 or 125

## Magnitude

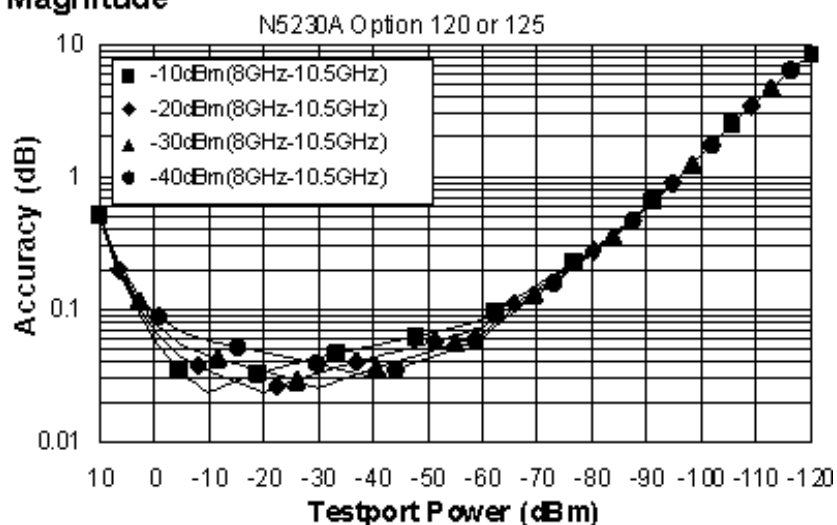


## Phase

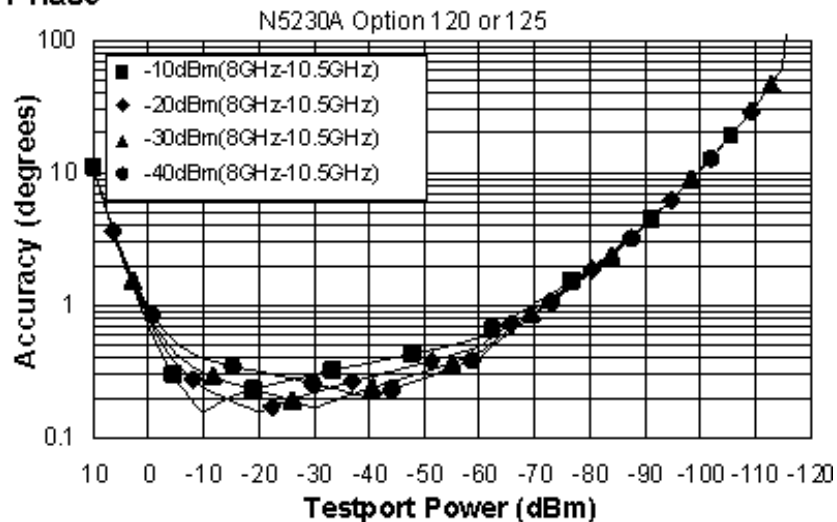


## Dynamic Accuracy, 10.5 - 12.5 GHz, Option 120 or 125

### Magnitude

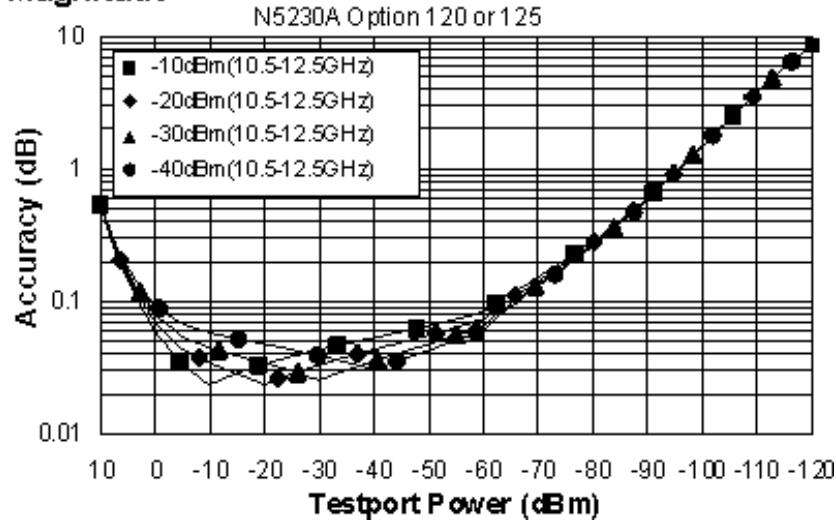


### Phase

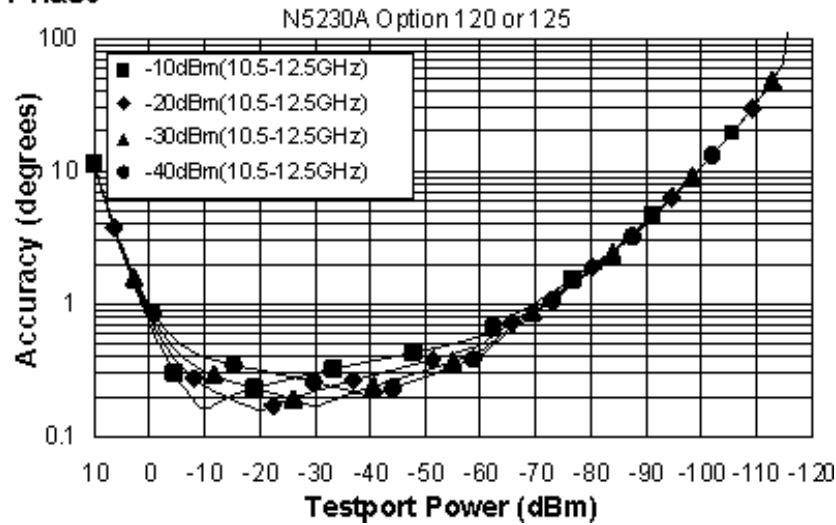


## Dynamic Accuracy, 12.5 - 13.5 GHz, Option 120 or 125

### Magnitude

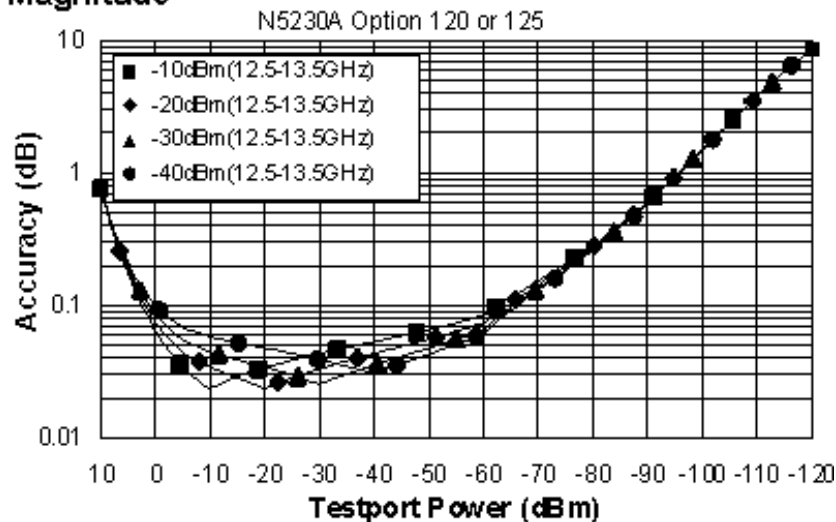


## Phase

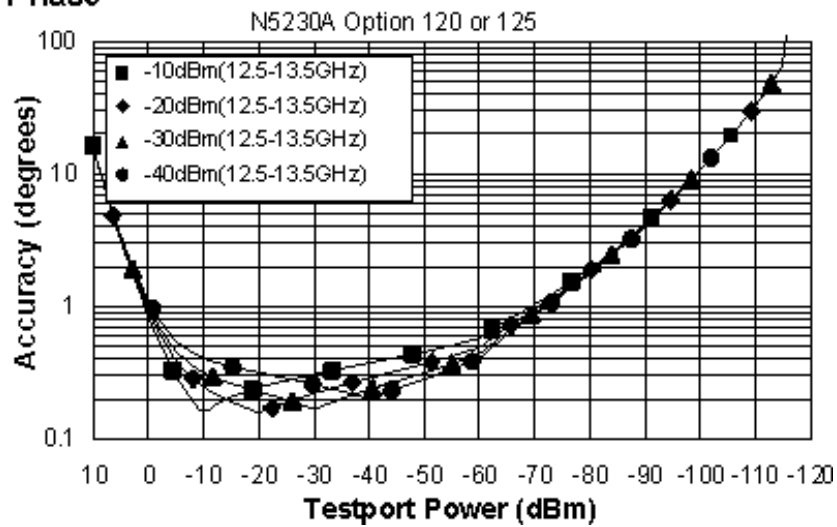


## Options 220, 225

Dynamic Accuracy, 0.045 GHz, Option 220 or 225


## Magnitude

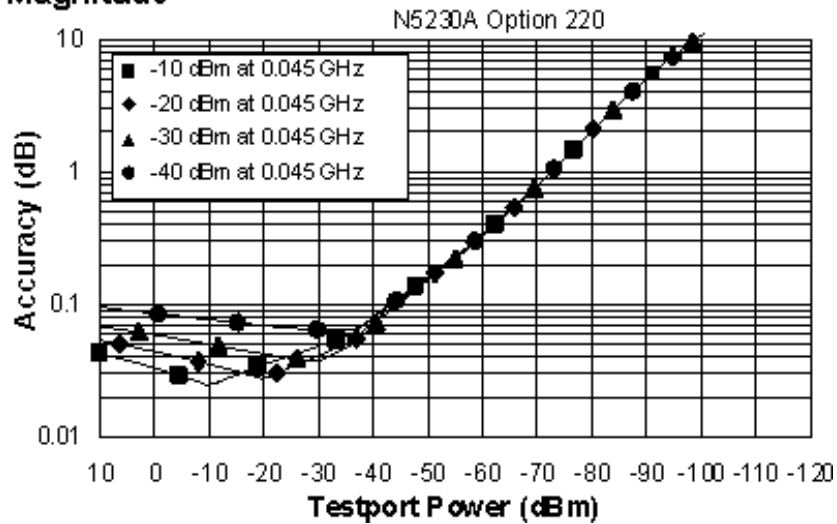


### Phase

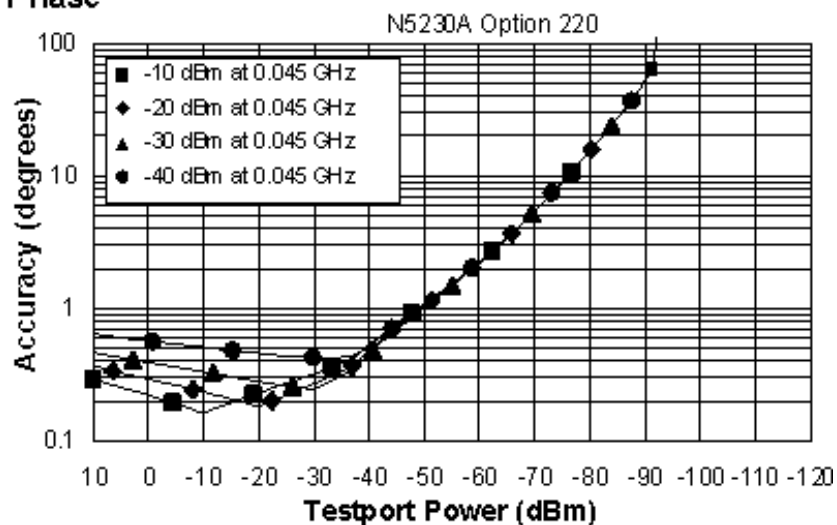

### Magnitude

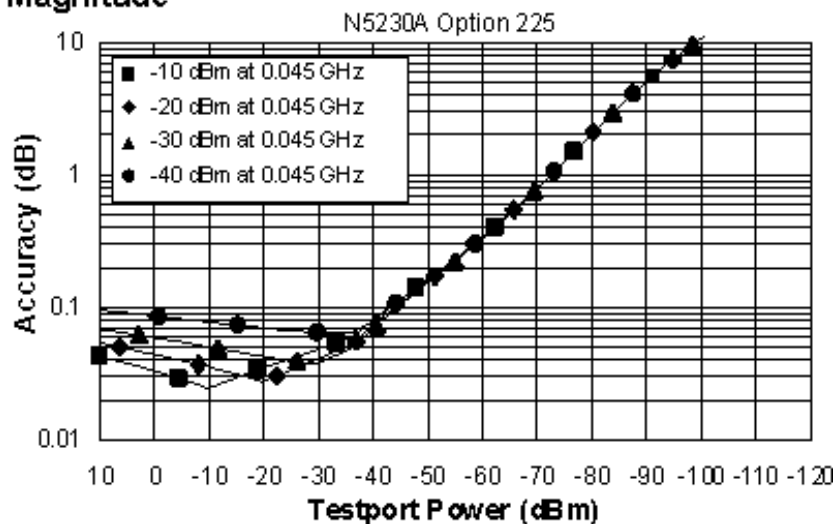


### Phase

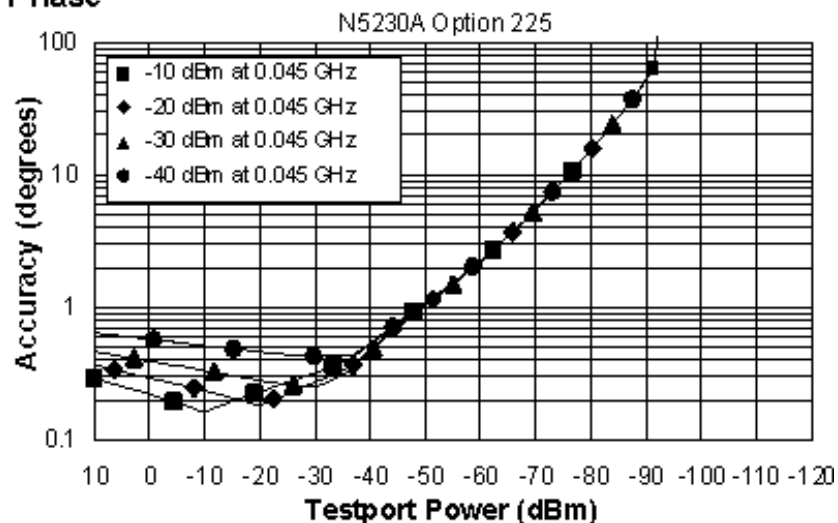


Dynamic Accuracy, 0.500 GHz, Option 220 or 225




### Magnitude

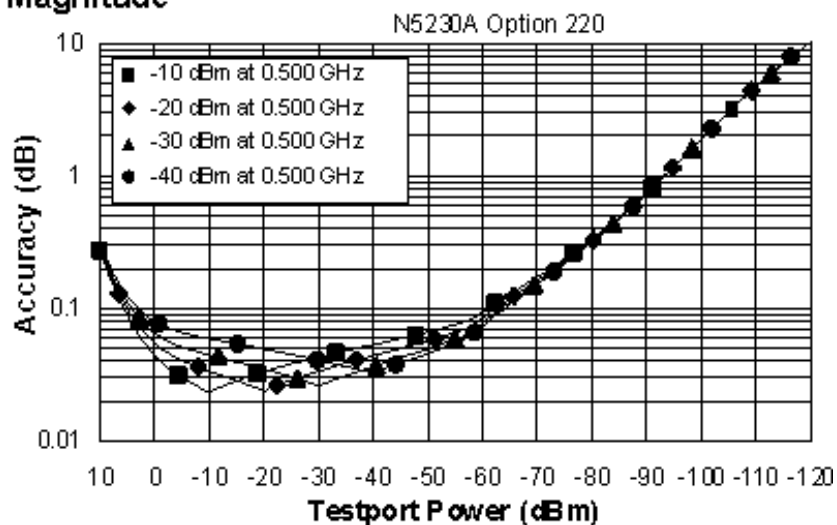


### Phase

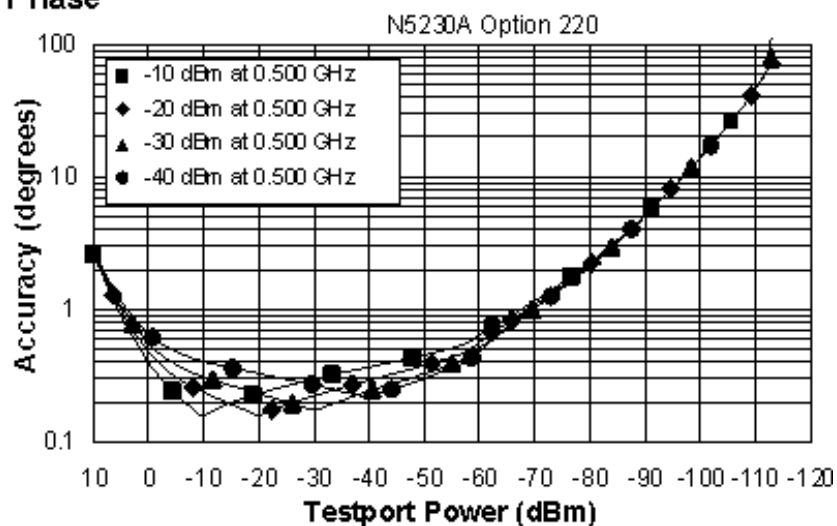

### Magnitude

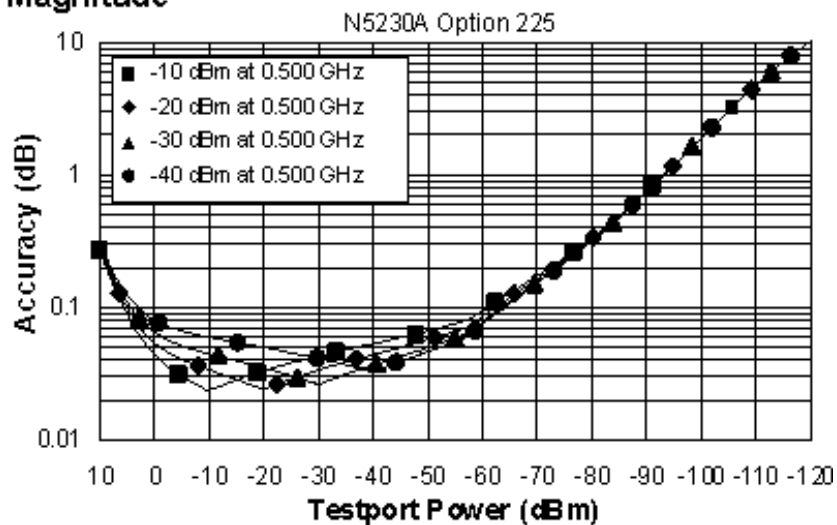


## Phase

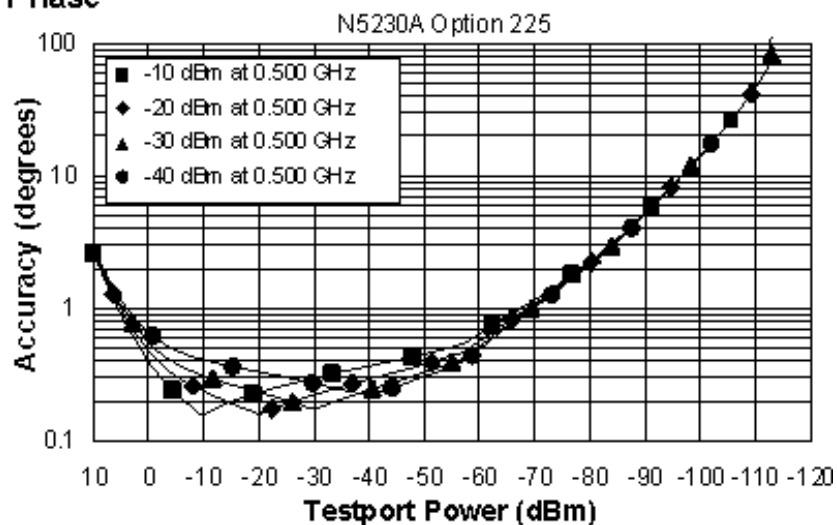


## Dynamic Accuracy, 0.500 - 2 GHz, Option 220 or 225


## Magnitude

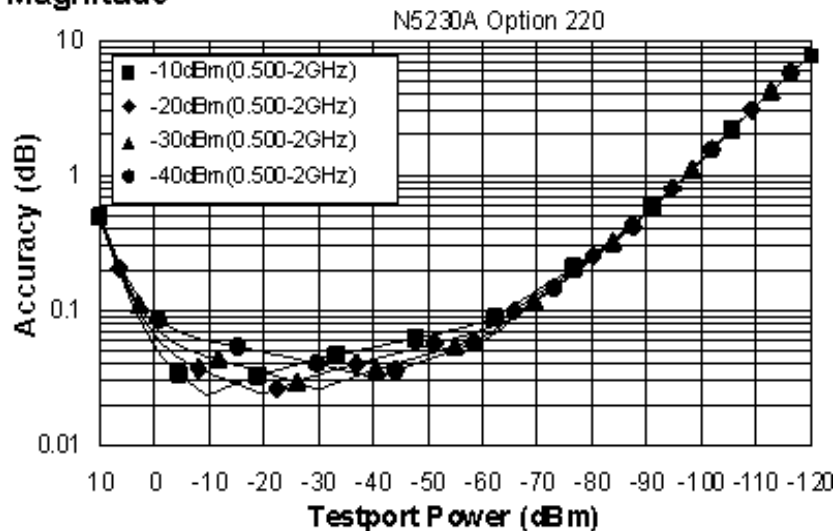


## Phase

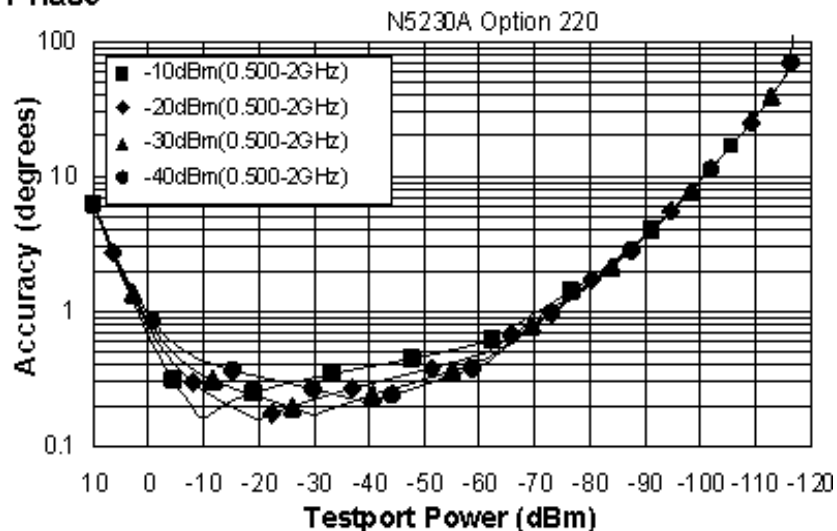

## Magnitude

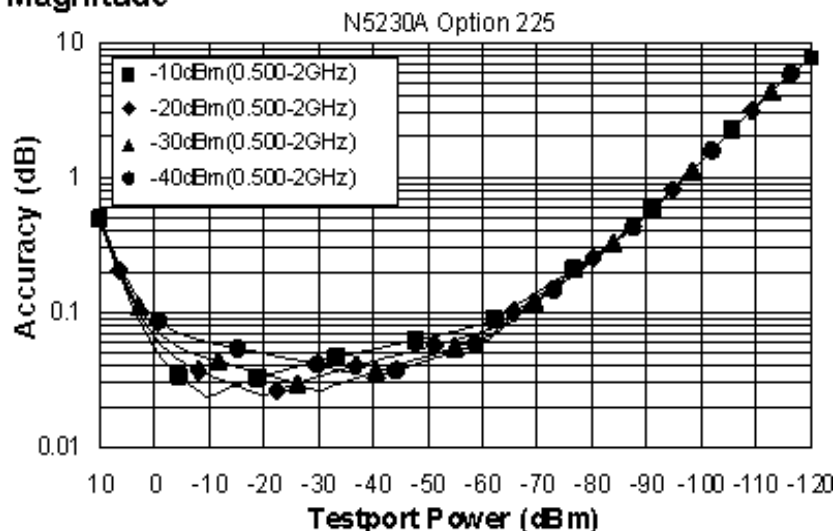


## Phase

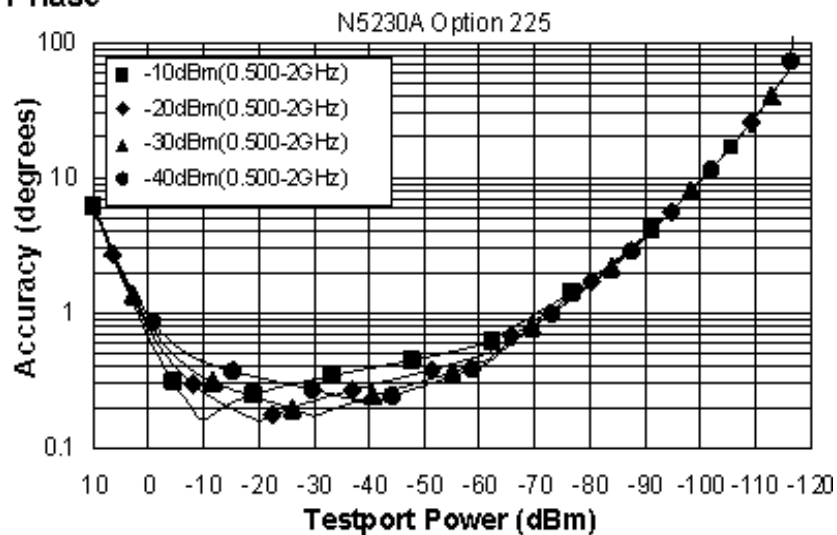


## Dynamic Accuracy, 2 - 12.5 GHz, Option 220 or 225


## Magnitude

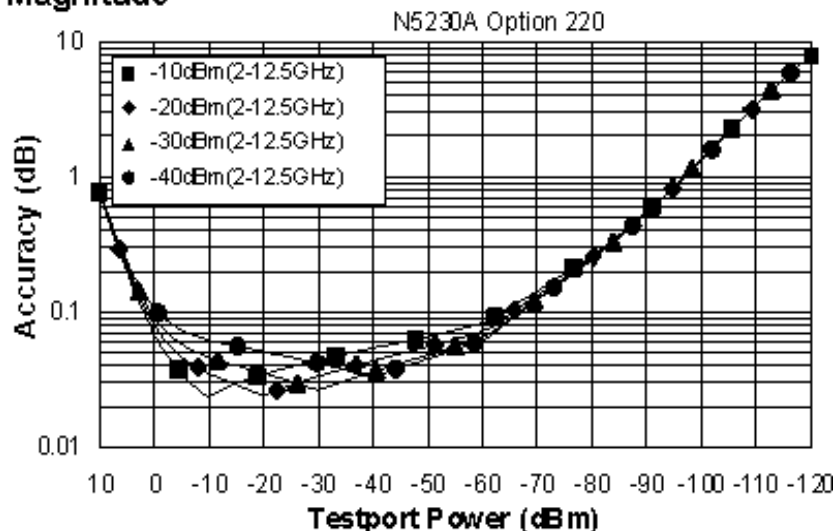


### Phase

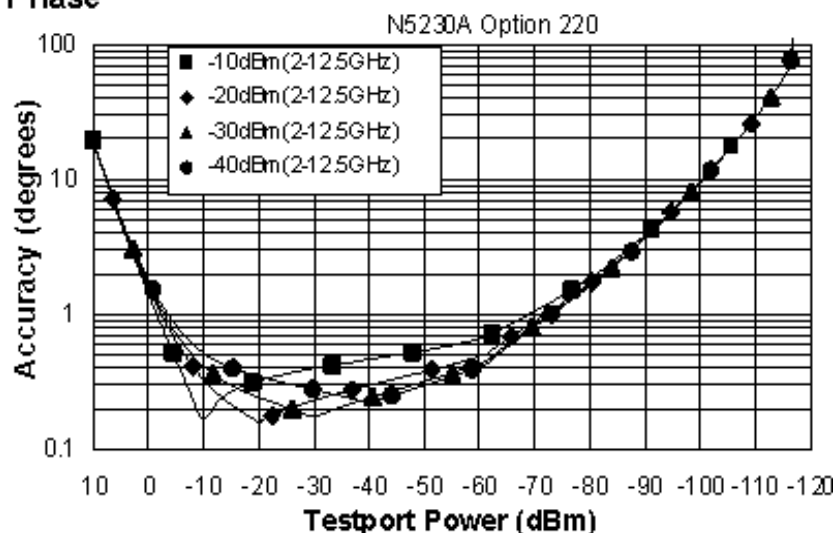

### Magnitude

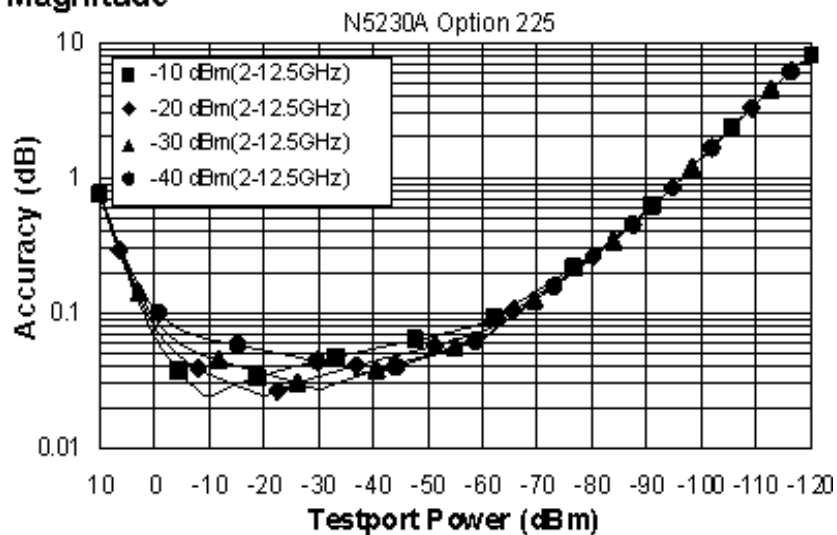


### Phase

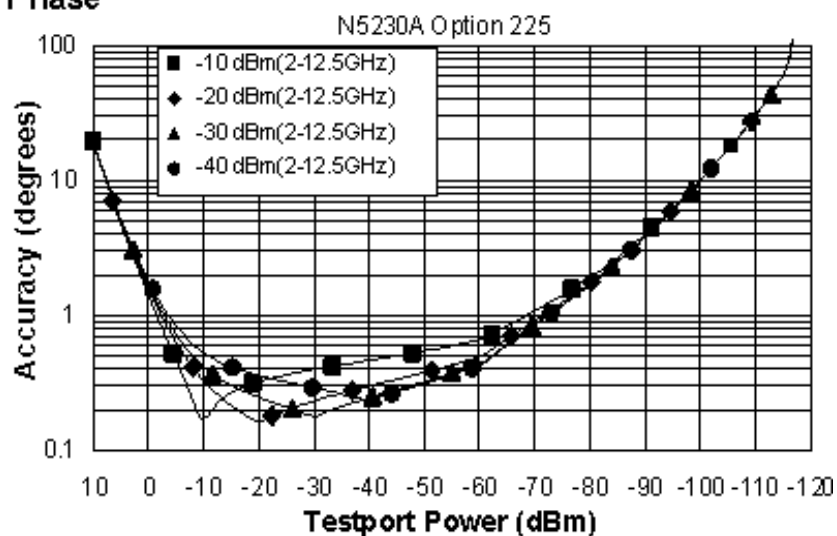


Dynamic Accuracy, 12.5 - 20 GHz, Option 220 or 225


### Magnitude

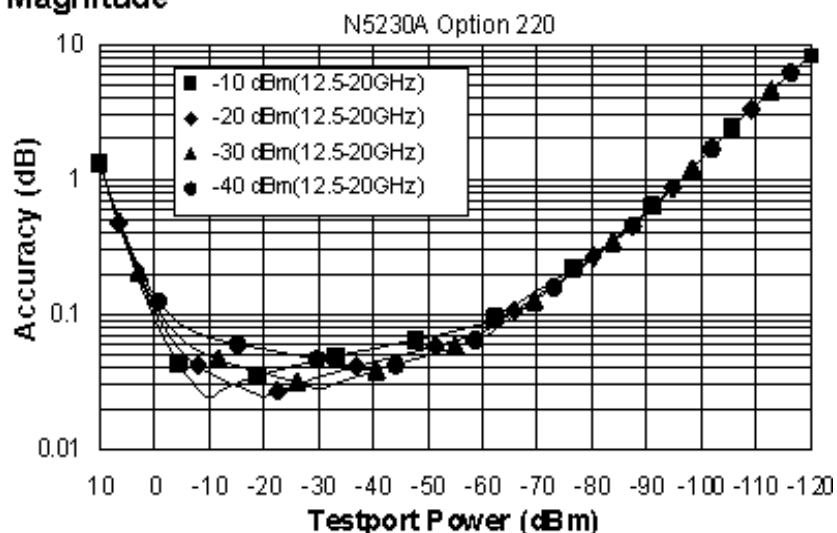


### Phase

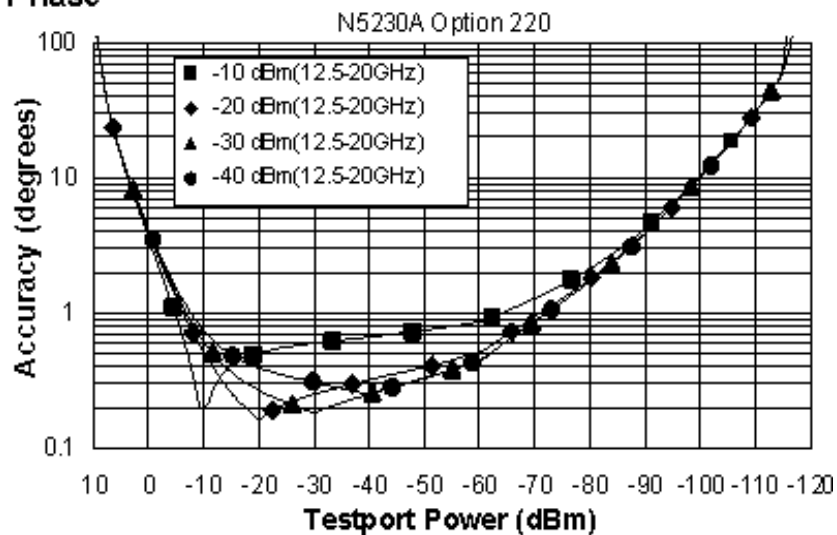

### Magnitude

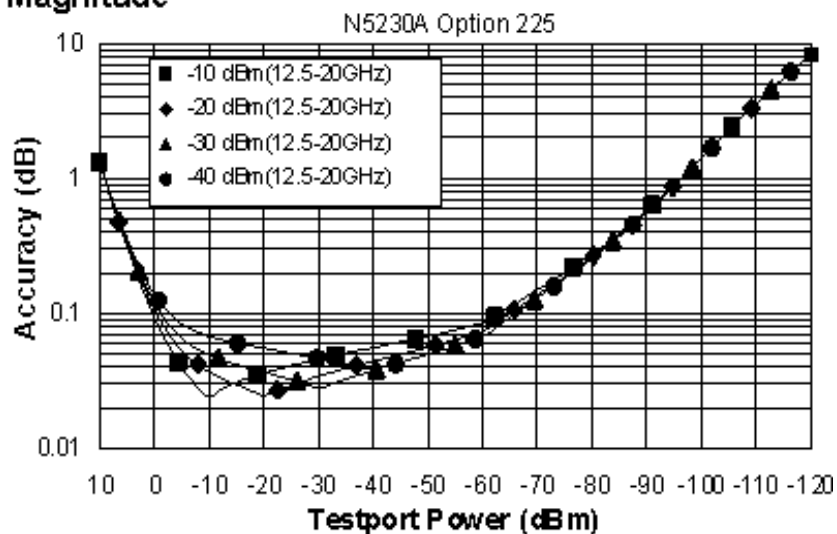


## Phase

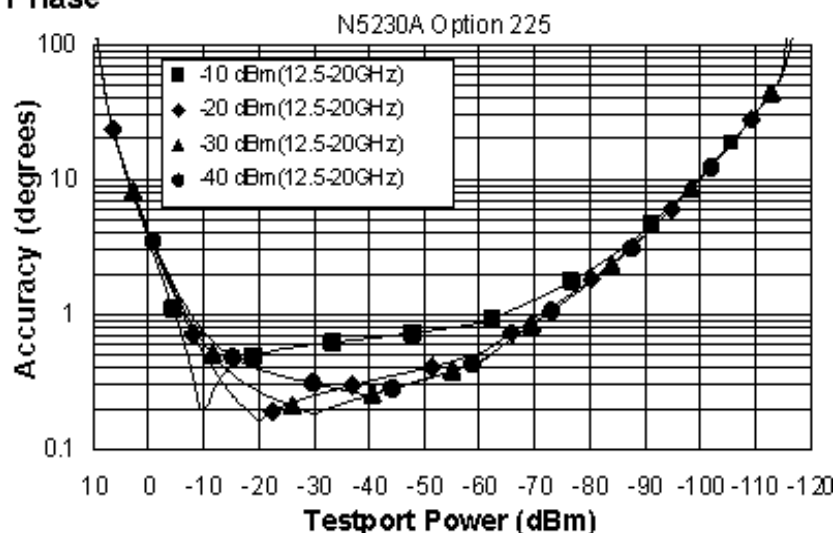


## Options 420, 425, 520, 525

Dynamic Accuracy, 0.045 GHz, Option 420, 425, 520, or 525


## Magnitude

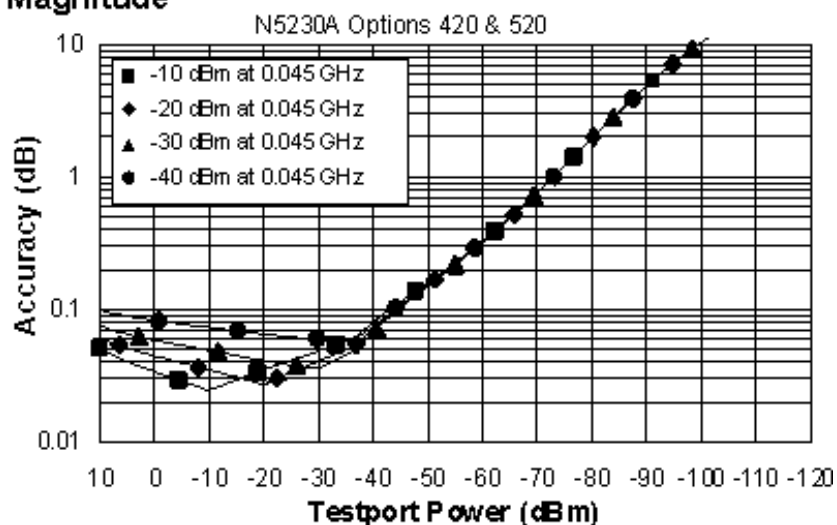


## Phase

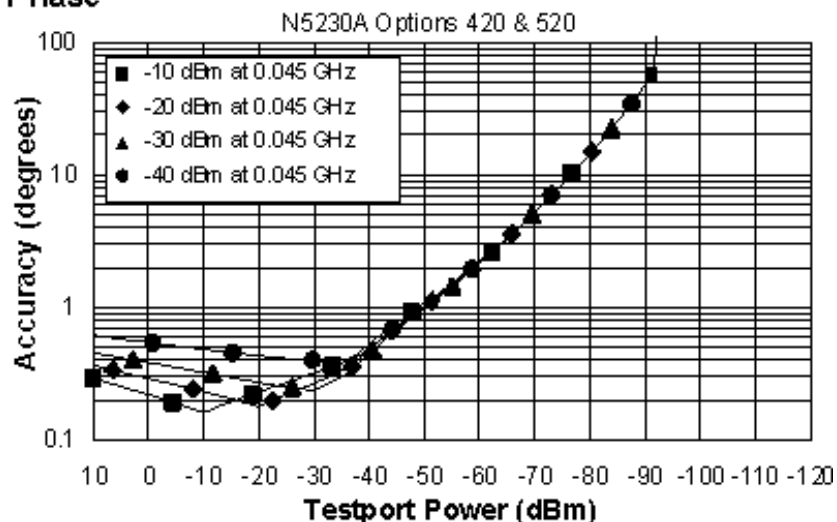

### Magnitude

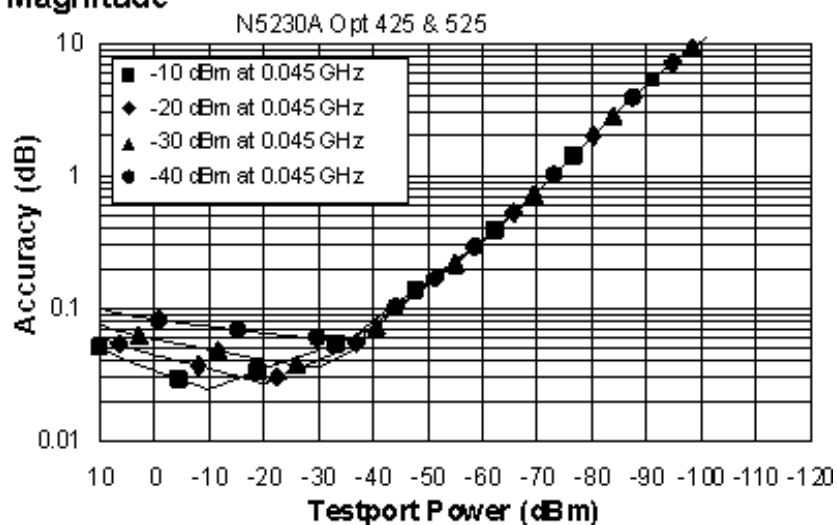


### Phase

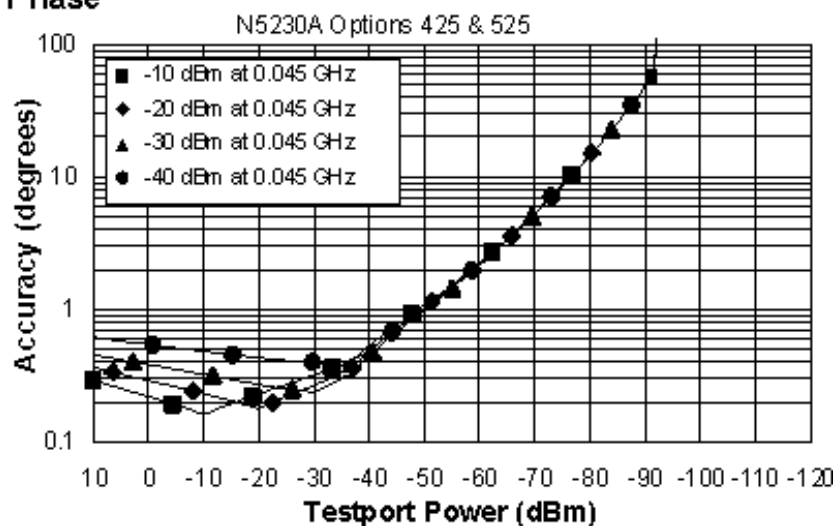


### Dynamic Accuracy, 0.500 GHz, Option 420, 425, 520, or 525


### Magnitude

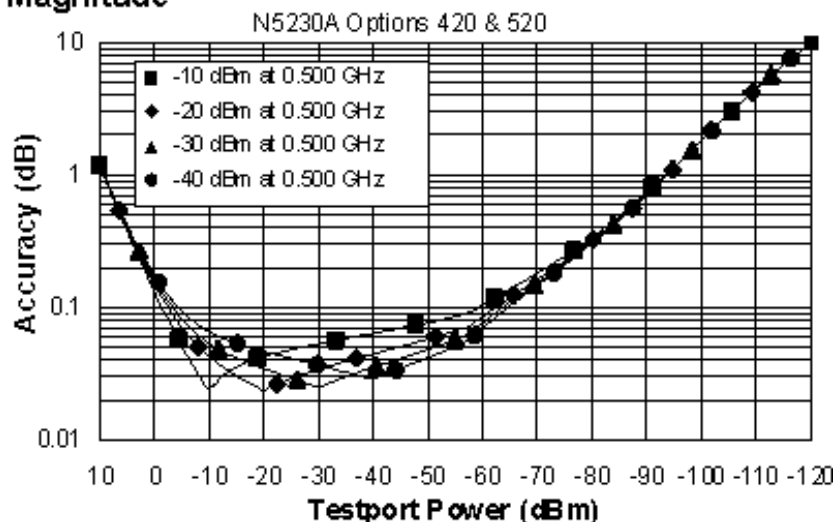


### Phase

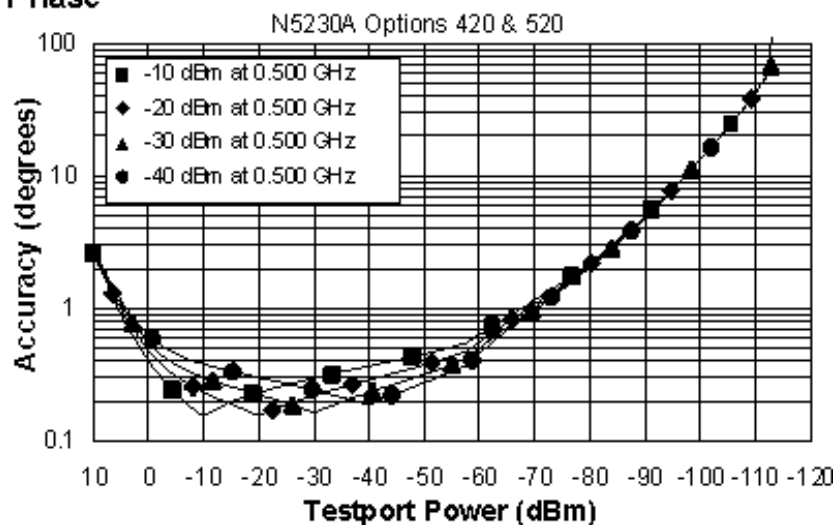

### Magnitude

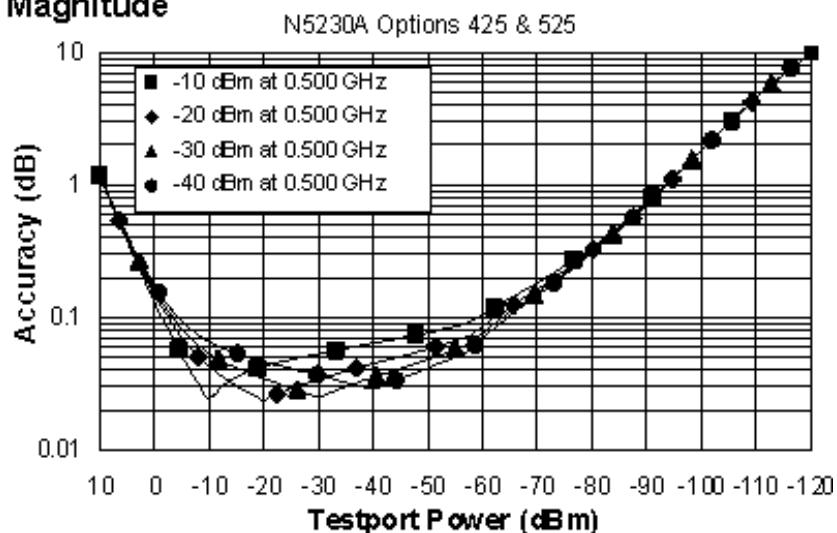


### Phase

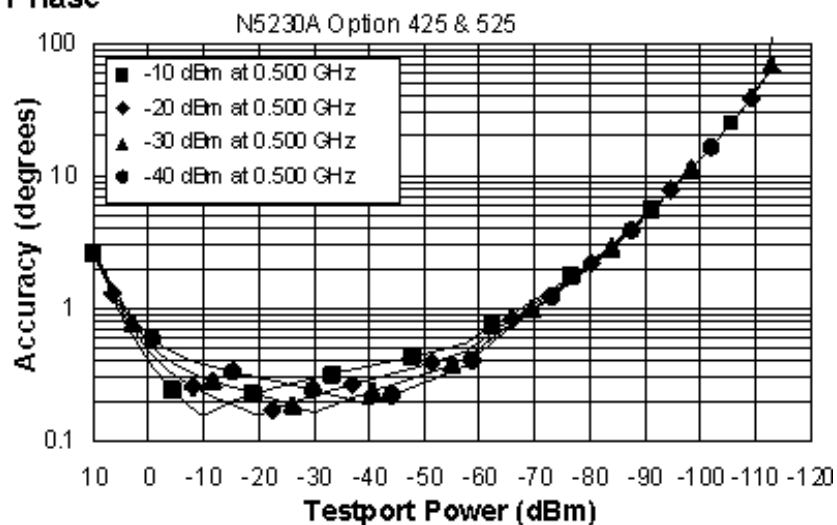


Dynamic Accuracy, 0.500 - 2 GHz, Option 420, 425, 520, or 525




### Magnitude

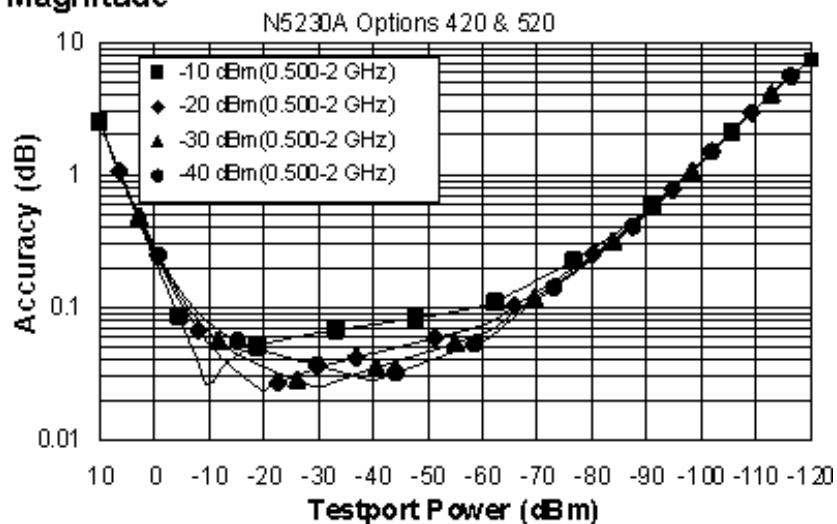


### Phase

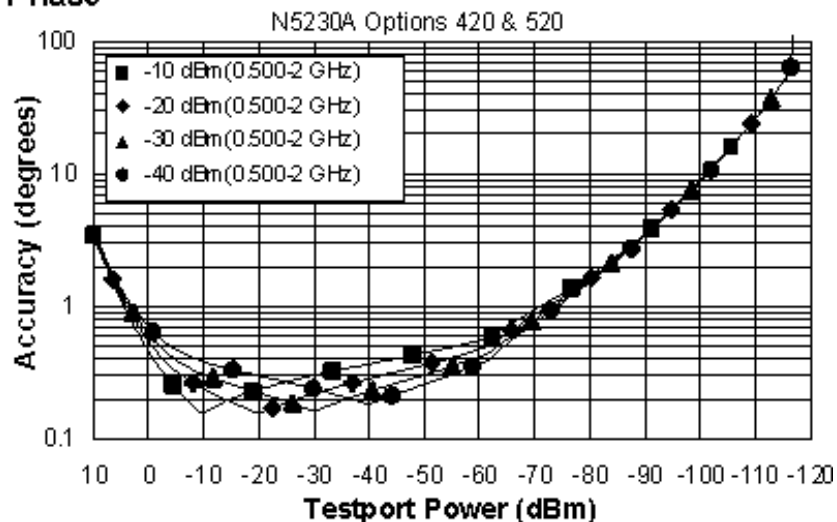

### Magnitude

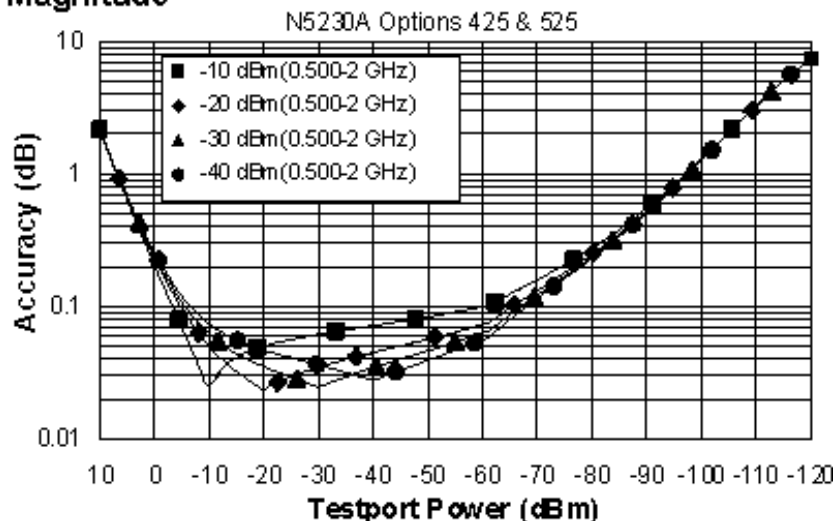


## Phase

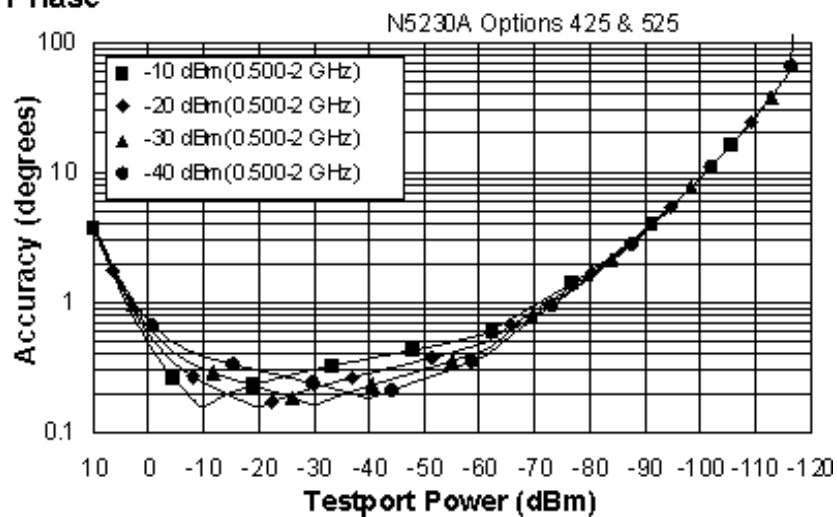


Dynamic Accuracy, 2 - 8 GHz, Option 420, 425, 520, or 525


## Magnitude

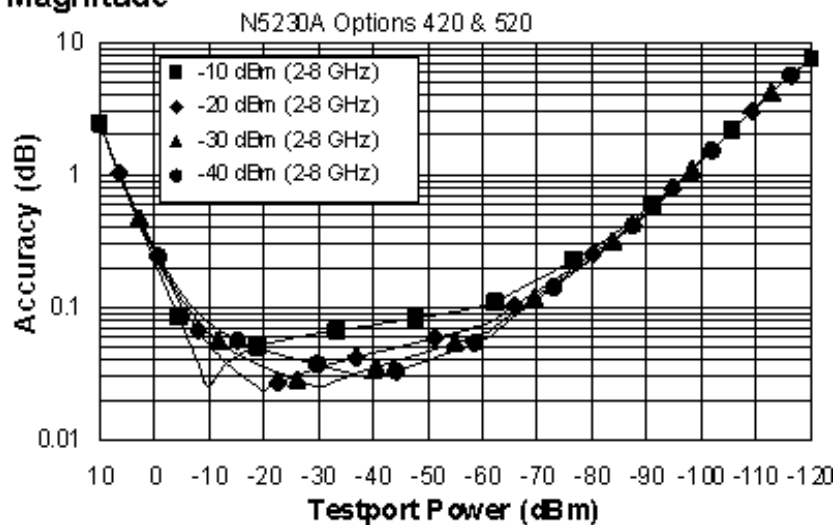


## Phase

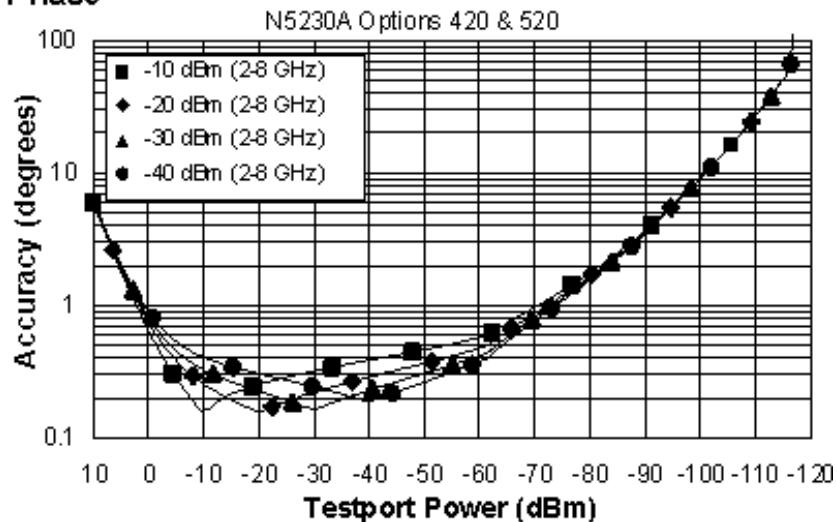

## Magnitude

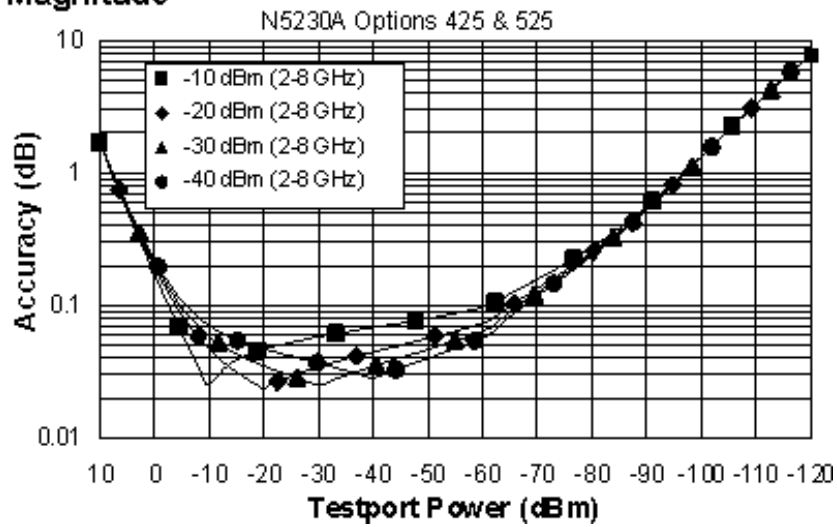


## Phase

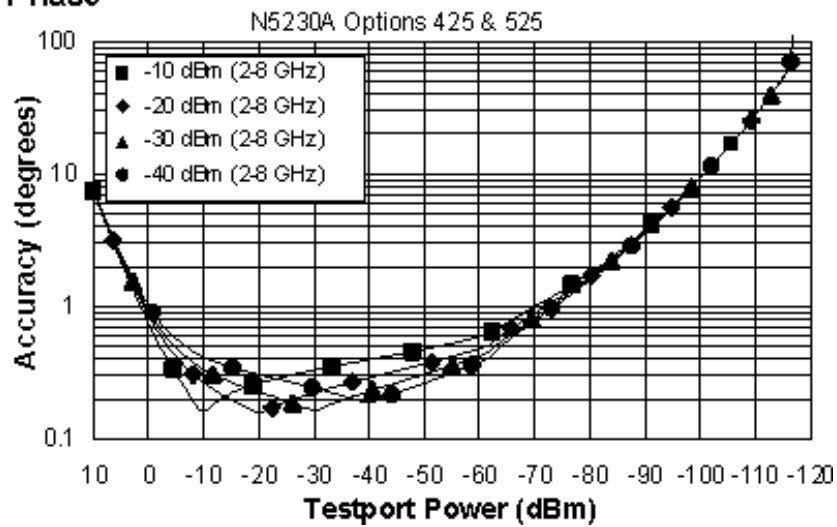


Dynamic Accuracy, 8 - 12.5 GHz, Option 420, 425, 520, or 525


### Magnitude

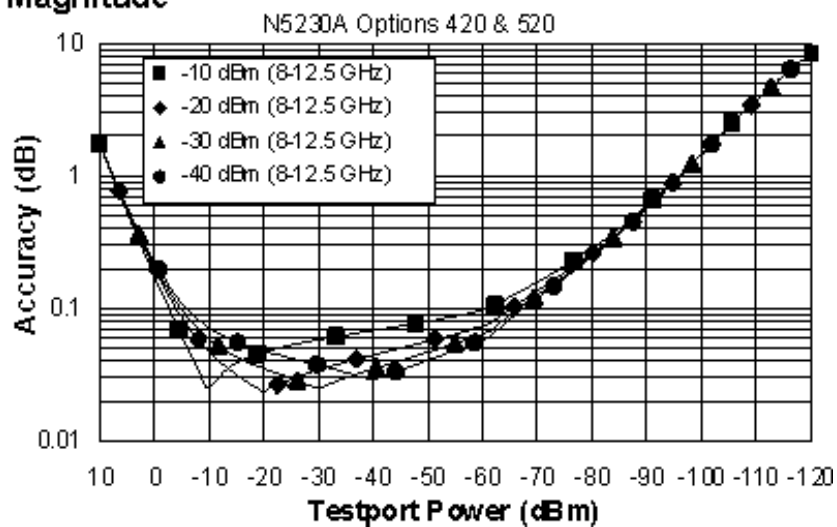


### Phase

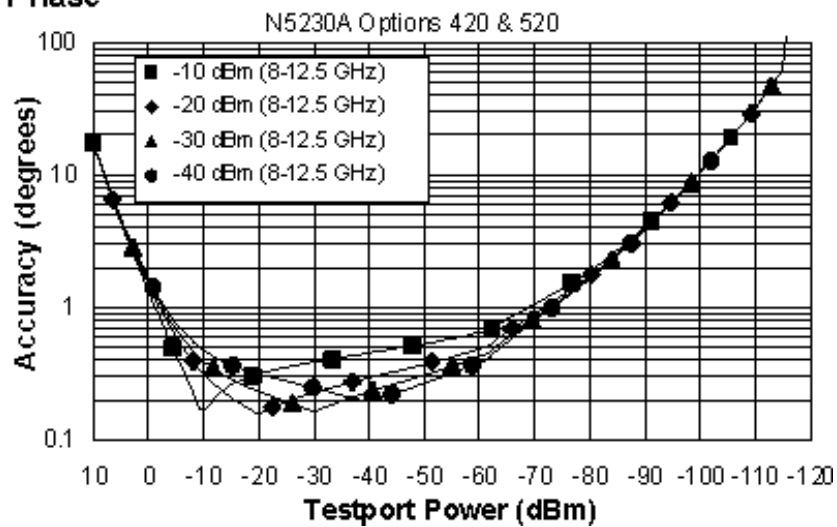

### Magnitude

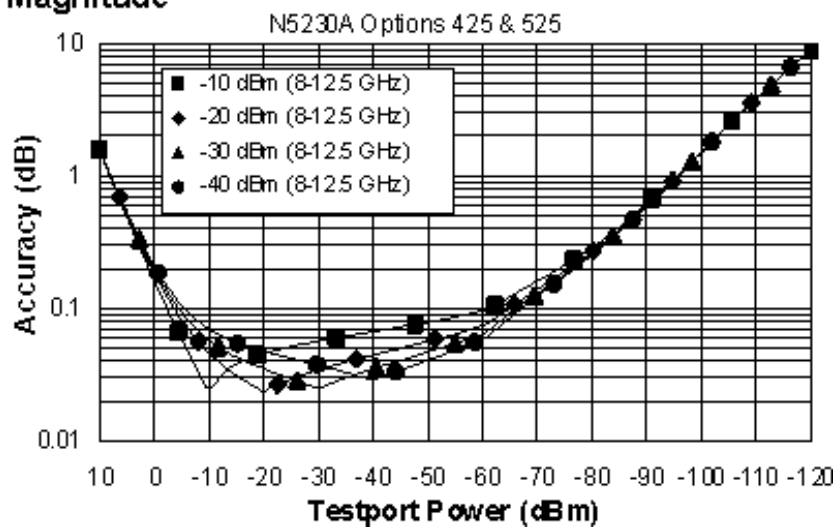


### Phase

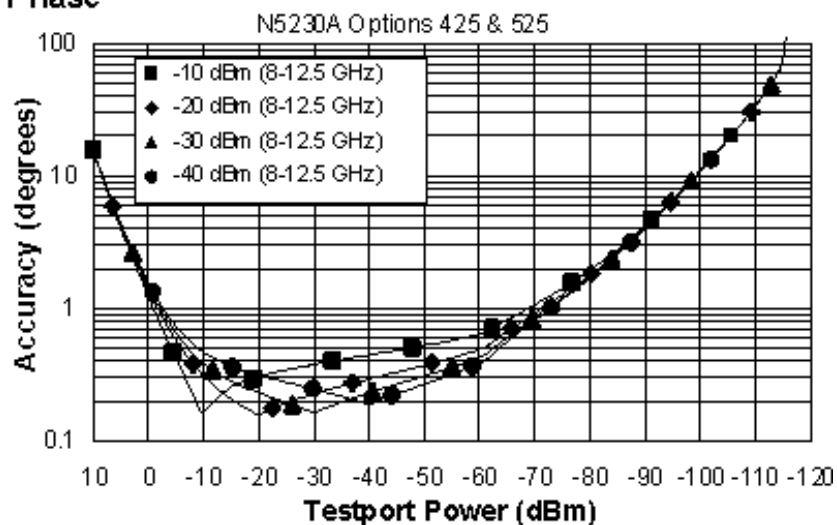


Dynamic Accuracy, 12.5 - 20 GHz, Option 420, 425, 520, or 525


### Magnitude

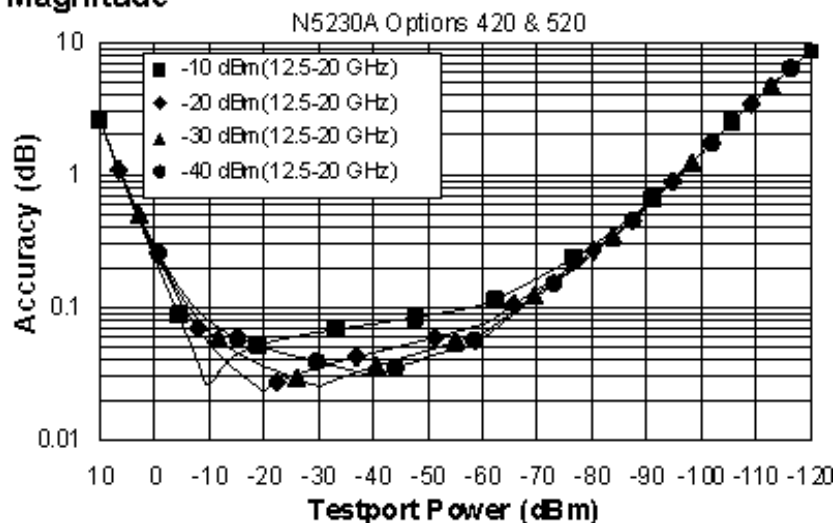


### Phase

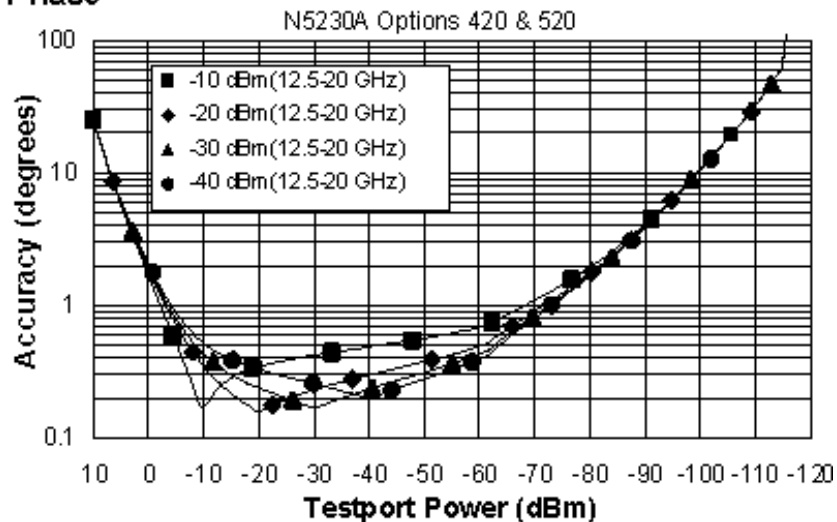

## Magnitude

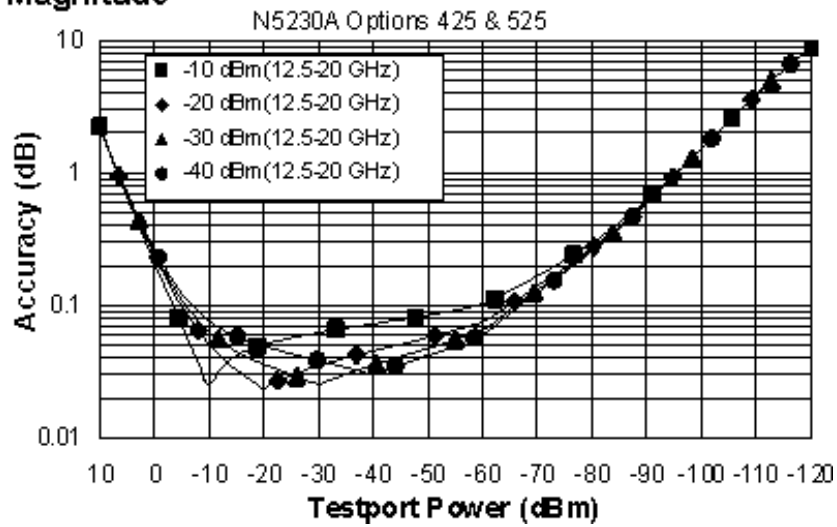


## Phase

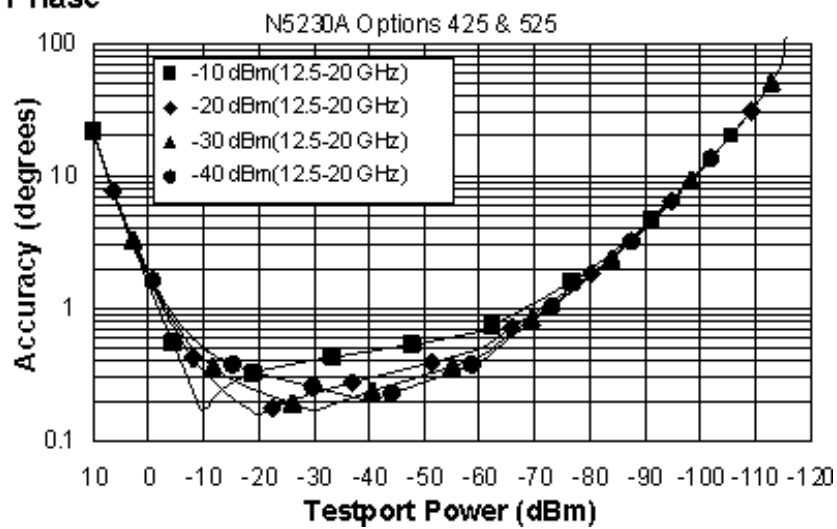


Dynamic Accuracy, 20 - 31.25 GHz, Option 420, 425, 520, or 525


### Magnitude

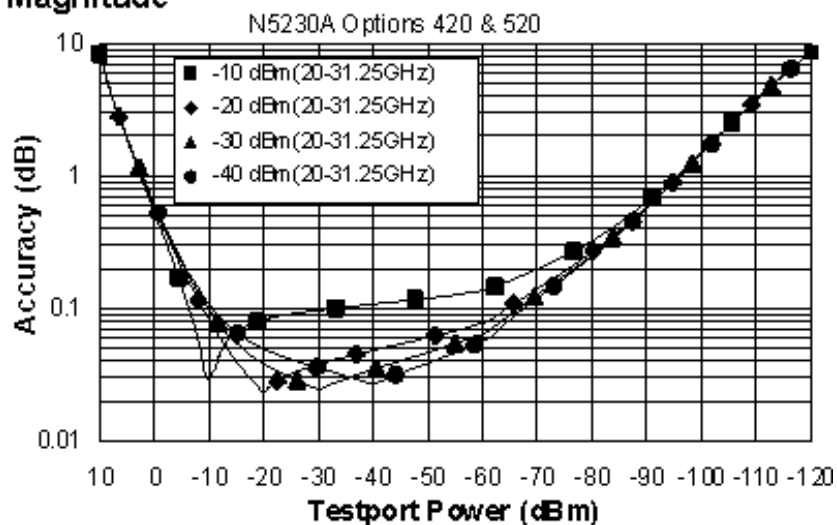


### Phase

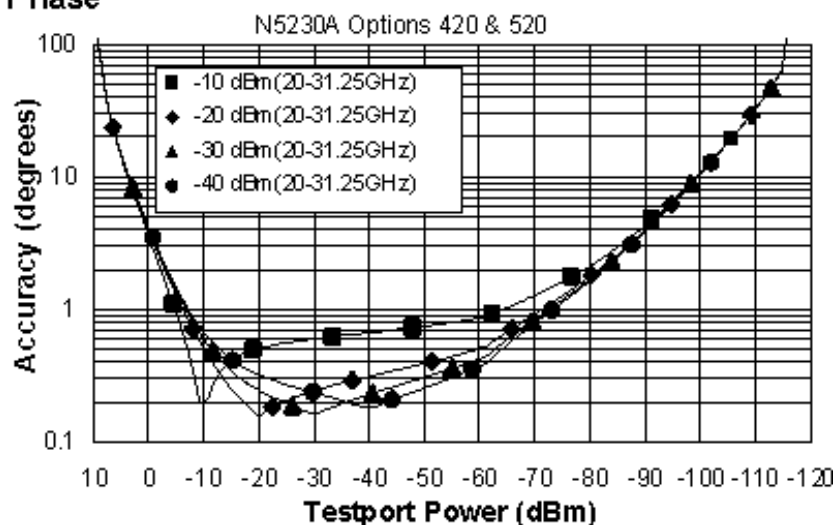

### Magnitude

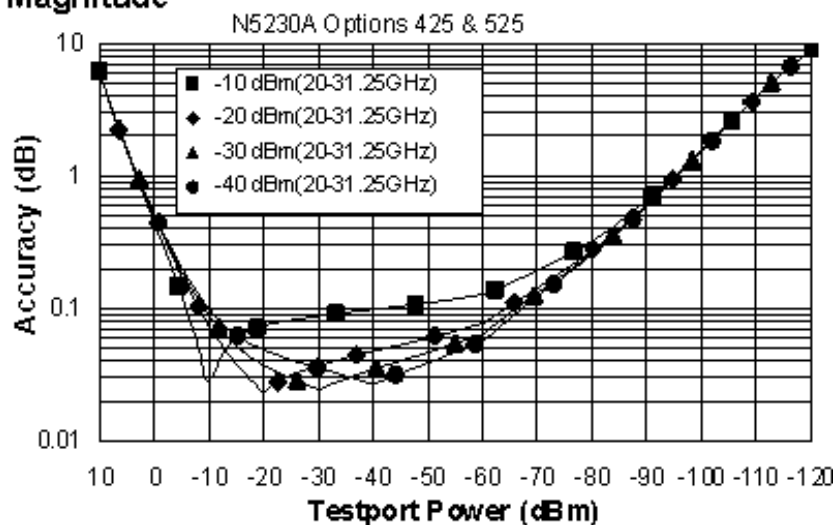


### Phase

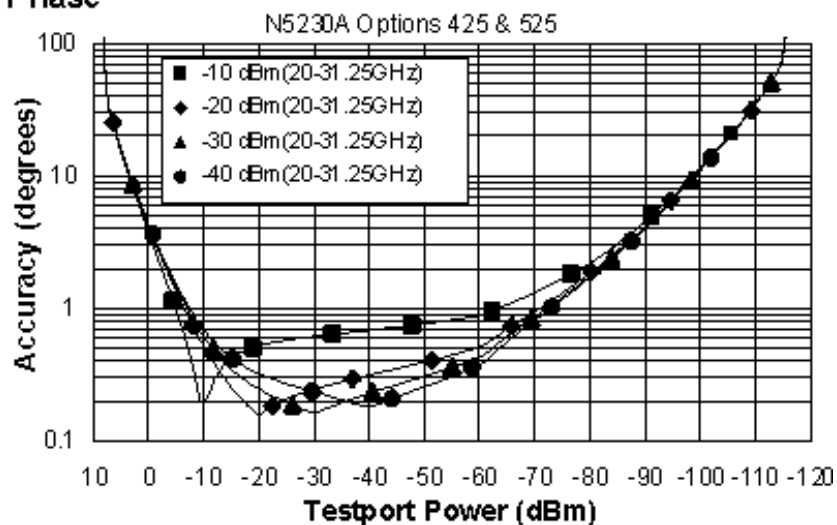


Dynamic Accuracy, 31.25 - 40 GHz, Option 420, 425, 520, or 525

### Magnitude

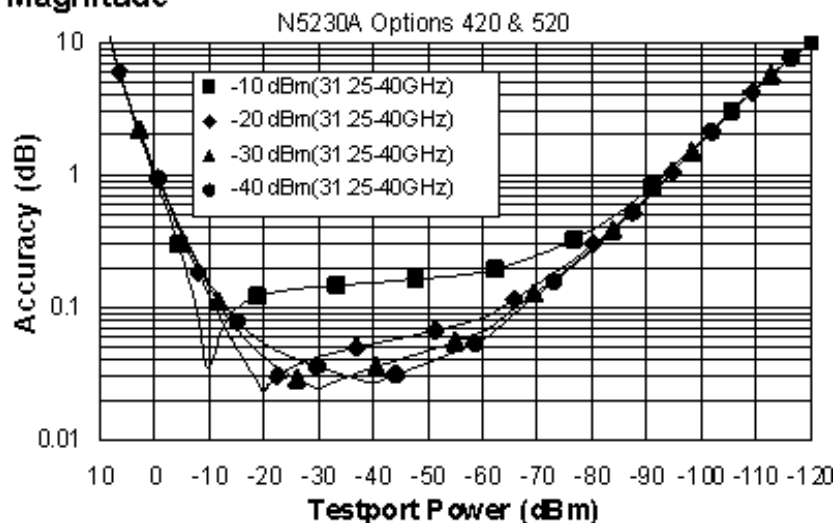


### Phase

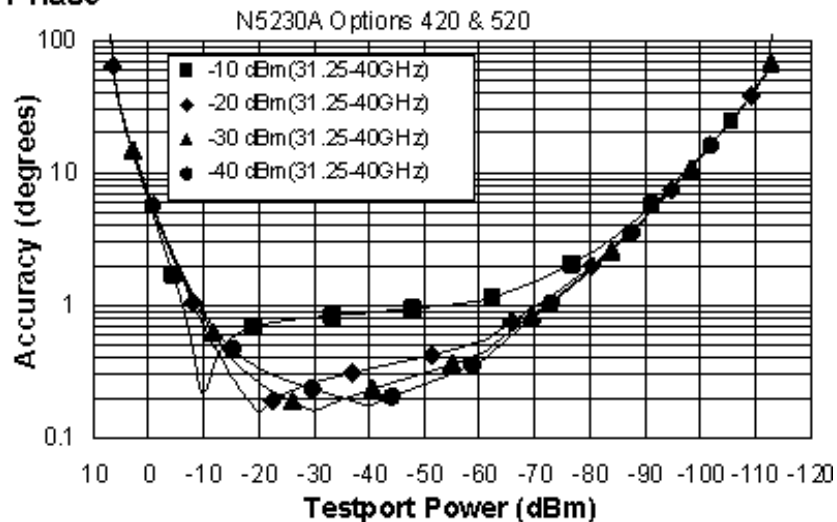




## Magnitude

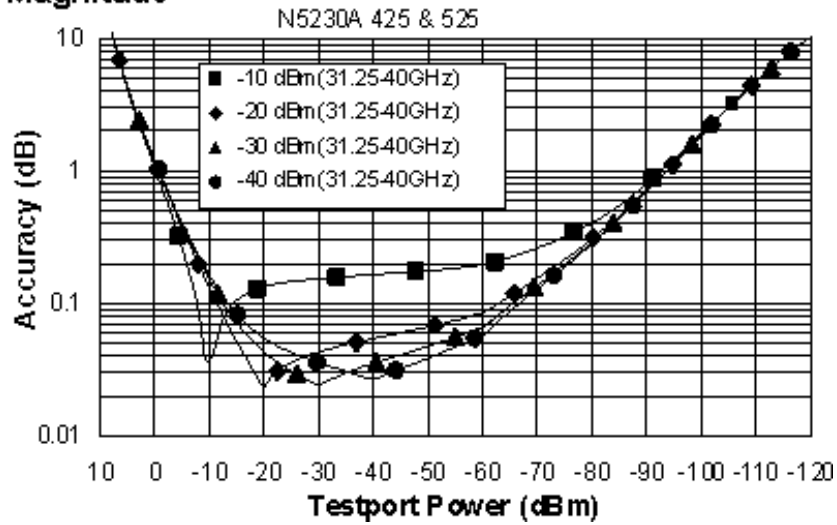


## Phase

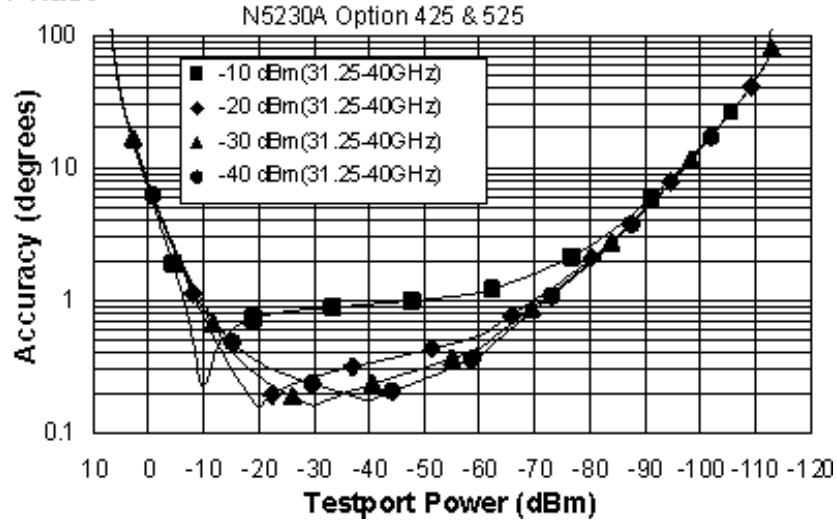


Dynamic Accuracy, 40 - 50 GHz, Option 520 or 525


### Magnitude

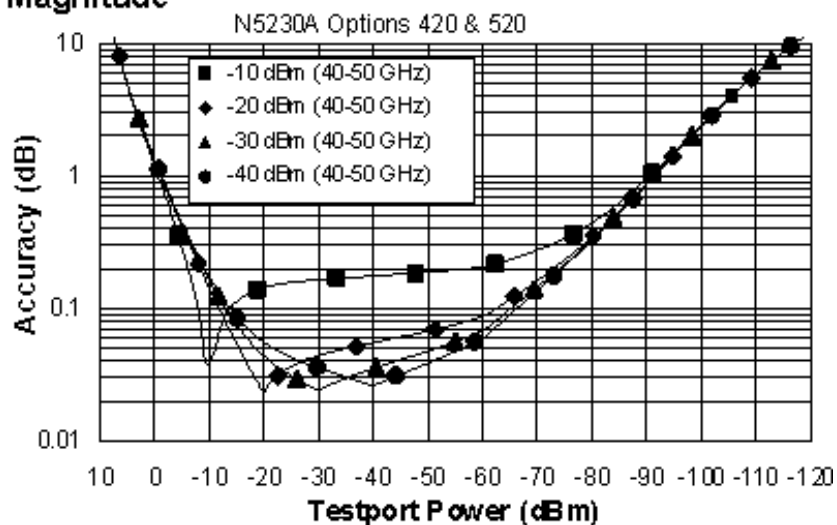


### Phase

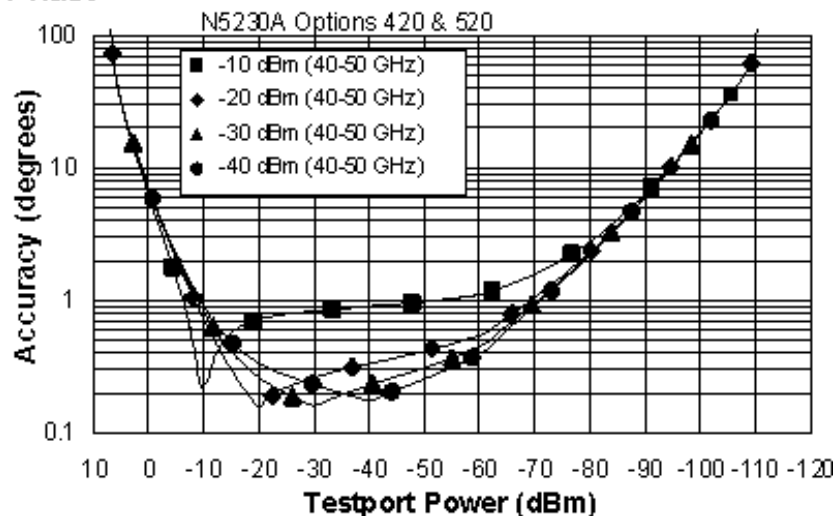

### Magnitude

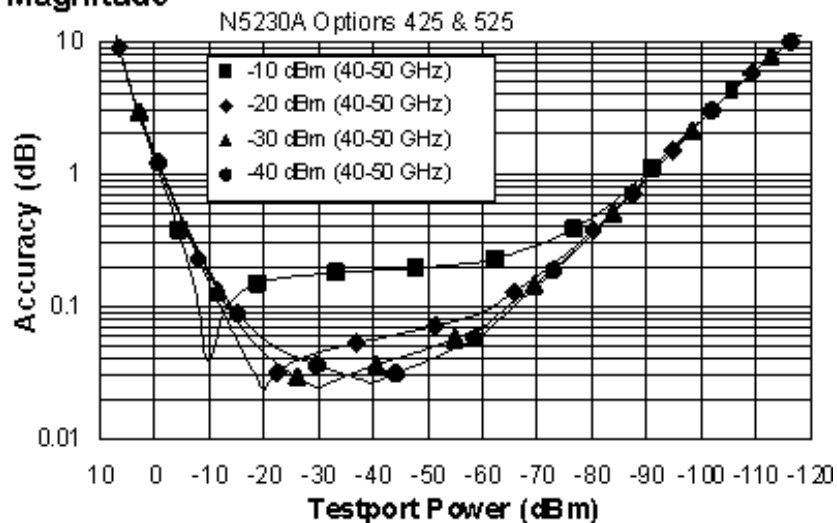

## Phase

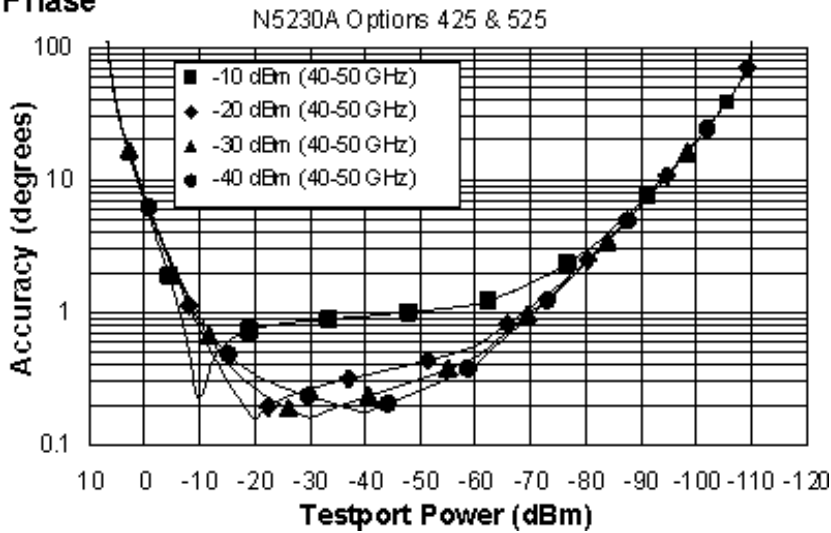

a Dynamic accuracy is verified with the following measurements:


- compression over frequency
- IF linearity at a single frequency of 1.195 GHz using a reference level of -20 dBm for an input power range of 0 to -110 dBm.

**Table 19. Test Port Input (Group Delay)<sup>a</sup>**

| Description           | Specification | Supplemental Information (typ.)                                                      |
|-----------------------|---------------|--------------------------------------------------------------------------------------|
| Aperture (selectable) |               | (frequency span)/(number of points -1)                                               |
| Maximum Aperture      |               | 20% of frequency span                                                                |
| Range                 |               | 0.5 x (1/minimum aperture)                                                           |
| Maximum Delay         |               | Limited to measuring no more than 180° of phase change within the minimum aperture.) |
| Accuracy              |               | See graph below. Char.                                                               |

The following graph shows characteristic group delay accuracy with full 2-port calibration and a 10 Hz IF bandwidth. Insertion loss is assumed to be < 2 dB and electrical length to be ten meters.

### Group Delay (Typical)

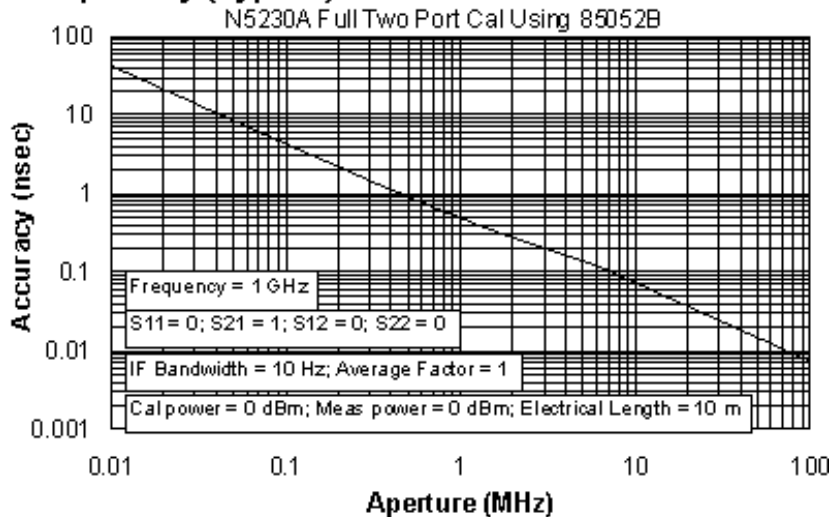

In general, the following formula can be used to determine the accuracy, in seconds, of specific group delay measurement:

$$\pm \text{Phase Accuracy (deg)} / [360 \times \text{Aperture (Hz)}]$$

Depending on the aperture and device length, the phase accuracy used is either incremental phase accuracy or worst case phase accuracy.

**a** Group delay is computed by measuring the phase change within a specified frequency step (determined by the frequency span and the number of points per sweep).

## General Information

[Miscellaneous Information](#)

[Front Panel](#)

[Rear Panel](#)

[Environment and Dimensions](#)

**Table 20.** Miscellaneous Information

| Description               | Specification | Supplemental Information    |
|---------------------------|---------------|-----------------------------|
| System IF Bandwidth Range |               | 1 Hz to 250 kHz, nominal    |
| CPU                       |               | Intel® 500 MHz Pentium® III |

**Table 21.** Front Panel Information

| Description          | Supplemental Information                                                                                              |
|----------------------|-----------------------------------------------------------------------------------------------------------------------|
| <b>RF Connectors</b> |                                                                                                                       |
| <b>N5230A</b>        |                                                                                                                       |
| Type                 | Option 220 or 225: 3.5 mm (male), 50 ohm, (nominal)<br>Option 420, 425, 520, or 525: 2.4 mm (male), 50 ohm, (nominal) |
| Center Pin Recession | 0.002 in. (characteristic)                                                                                            |
| <b>Display</b>       |                                                                                                                       |
| Size                 | 21.3 cm (8.4 in) diagonal color active matrix LCD; 640 (horizontal) X 480 (vertical) resolution                       |
| Refresh Rate         | Vertical 59.83 Hz; Horizontal 31.41 kHz                                                                               |

|                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
|---------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Pixels                    | <p>When running the analyzer's built-in "Display Test<sup>1</sup>," one or more of the following symptoms indicate a faulty display assembly:</p> <ul style="list-style-type: none"> <li>• A complete row or column of "stuck on" or "dark" pixels.</li> <li>• More than six "stuck on" pixels (but not more than three green)</li> <li>• More than twelve "dark" pixels (but not more than seven of the same color)</li> <li>• Two or more consecutive "stuck on" pixels or three or more consecutive "dark" pixels (but no more than one set of two consecutive dark pixels)</li> <li>• "Stuck on" or "dark" pixels less than 6.5 mm apart (excluding consecutive pixels)</li> </ul> |
| <b>Display Range</b>      |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| Magnitude                 | ±500 dB (at 20 dB/div), max                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| Phase                     | ±500°, max                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| Polar                     | 10 pUnits, min<br>1000 Units, max                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>Display Resolution</b> |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| Magnitude                 | 0.001 dB/div, min                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| Phase                     | 0.01°/div, min                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Marker Resolution</b>  |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| Magnitude                 | 0.001 dB, min                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| Phase                     | 0.01°, min                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| Polar                     | 0.01 mUnit, min; 0.01°, min                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |

1 Any PNA Service Guide contains instructions for running the analyzer's built-in "Display Test." You can view a PDF file of a Service Guide on the CD-ROM that you received with your PNA, or on the Web at <http://www.agilent.com>. After opening the PDF file, look in the left-side column and click on the "Index" bookmark. From the index, click on "Display Test".

**Table 22.** Rear Panel Information

| Description                 | Supplemental Information    |
|-----------------------------|-----------------------------|
| <b>10 MHz Reference In</b>  |                             |
| Connector                   | BNC, female                 |
| Input Frequency             | 10 MHz ± 10 ppm, Typical    |
| Input Level                 | -15 dBm to +20 dBm, Typical |
| Input Impedance             | 200 Ω, nom.                 |
| <b>10 MHz Reference Out</b> |                             |
| Connector                   | BNC, female                 |

|                             |                                                                                                                                                                                                                    |
|-----------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Output Frequency            | 10 MHz $\pm$ 1 ppm, Typical                                                                                                                                                                                        |
| Signal Type                 | Sine Wave, Typical                                                                                                                                                                                                 |
| Output Level                | +10 dBm $\pm$ 4 dB into 50 $\Omega$ , Typical                                                                                                                                                                      |
| Output Impedance            | 50 $\Omega$ , nominal                                                                                                                                                                                              |
| Harmonics                   | <-40 dBc, Typical                                                                                                                                                                                                  |
| <b>VGA Video Output</b>     |                                                                                                                                                                                                                    |
| Connector                   | 15-pin mini D-Sub; Drives VGA compatible monitors                                                                                                                                                                  |
| Devices Supported:          |                                                                                                                                                                                                                    |
|                             | <b>Resolutions:</b>                                                                                                                                                                                                |
| Flat Panel (TFT)            | 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                                   |
| Flat Panel (DSTN)           | 800 X 600, 640 X 480                                                                                                                                                                                               |
| CRT Monitor                 | 1280 X 1024, 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                      |
|                             | Simultaneous operation of the internal and external displays is allowed, but with 640 X 480 resolution only. If you change resolution, you can only view the external display (internal display will "white out"). |
| <b>Test Set IO</b>          |                                                                                                                                                                                                                    |
|                             | 25-pin D-Sub connector, available for external test set control                                                                                                                                                    |
| <b>Aux IO</b>               |                                                                                                                                                                                                                    |
|                             | 25-pin D-Sub connector, male, analog and digital IO                                                                                                                                                                |
| <b>Handler IO</b>           |                                                                                                                                                                                                                    |
|                             | 36-pin parallel I/O port; all input/output signals are default set to negative logic; can be reset to positive logic via GPIB command                                                                              |
| <b>GPIB</b>                 |                                                                                                                                                                                                                    |
|                             | 24-pin D-sub (Type D-24), female; compatible with IEEE-488.                                                                                                                                                        |
| <b>Parallel Port (LPT1)</b> |                                                                                                                                                                                                                    |
|                             | 25-pin D-Sub miniature connector, female; provides connection to printers or any other parallel port peripherals                                                                                                   |
| <b>Serial Port (COM 1)</b>  |                                                                                                                                                                                                                    |
|                             | 9-pin D-Sub, male; compatible with RS-232                                                                                                                                                                          |
| <b>USB Port</b>             |                                                                                                                                                                                                                    |
|                             | One port on front panel and five ports on rear panel. Universal Serial Bus jack, Type A configuration (4 contacts inline, contact 1 on left); female                                                               |

|           |                                        |
|-----------|----------------------------------------|
| Contact 1 | Vcc: 4.75 to 5.25 VDC, 500 mA, maximum |
| Contact 2 | -Data                                  |
| Contact 3 | +Data                                  |
| Contact 4 | Ground                                 |

**Table 22.** Rear Panel Information (Continued)

| Description                   | Supplemental Information                                                           |
|-------------------------------|------------------------------------------------------------------------------------|
| <b>LAN</b>                    |                                                                                    |
|                               | 10/100BaseT Ethernet, 8-pin configuration; auto selects between the two data rates |
| <b>Line Power<sup>1</sup></b> |                                                                                    |
| Frequency                     | 48 Hz to 66 Hz                                                                     |
| Voltage at 115 V Setting      | 90 to 132 VAC; 120 VAC, nominal                                                    |
| Voltage at 220 V Setting      | 198 to 264 VAC; 240 VAC, nominal                                                   |
| VA Max                        | 600 VA maximum                                                                     |

<sup>1</sup> A third-wire ground is required.

**Note:** Option H08 and Option H11 are not available with the N5230A

**Table 23.** Analyzer Environment and Dimensions

| Description                       | Supplemental Information                                                                                                                                                                                                                                 |
|-----------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>General Environmental</b>      |                                                                                                                                                                                                                                                          |
| RFI/EMI Susceptibility            | Defined by CISPR Pub. 11, Group 1, Class A, and IEC 50082-1                                                                                                                                                                                              |
| ESD                               | Minimize using static-safe work procedures and an antistatic bench mat                                                                                                                                                                                   |
| Dust                              | Minimize for optimum reliability                                                                                                                                                                                                                         |
| <b>Operating Environment</b>      |                                                                                                                                                                                                                                                          |
| Temperature                       | 0 °C to +40 °C<br><br>Instrument powers up and displays no error messages within this temperature range (except for "source unlevelled" error message that may occur at temperatures outside the specified performance temperature range of 25 +/- 5°C). |
| Error-Corrected Temperature Range | 23°C ± 3°C<br>with less than 1°C deviation from calibration temp.                                                                                                                                                                                        |
| Humidity                          | 5% to 95% at +40 °C                                                                                                                                                                                                                                      |

|                                          |                                      |
|------------------------------------------|--------------------------------------|
| Altitude                                 | 0 to 4500 m (14,760 ft.)             |
| <b>Non-Operating Storage Environment</b> |                                      |
| Temperature                              | -40 °C to +70 °C                     |
| Humidity                                 | 0% to 90% at +65 °C (non-condensing) |
| Altitude                                 | 0 to 15,240 m (50,000 ft.)           |

| <b>Cabinet Dimensions</b>                                                   |                   |                    |                    |
|-----------------------------------------------------------------------------|-------------------|--------------------|--------------------|
|                                                                             | <b>Height</b>     | <b>Width</b>       | <b>Depth</b>       |
| Excluding front and rear panel hardware and feet                            | 267 mm<br>10.5 in | 426 mm<br>16.75 in | 427 mm<br>16.8 in  |
| As shipped - includes front panel connectors, rear panel bumpers, and feet. | 280 mm<br>11.0 in | 435 mm<br>17.1 in  | 470 mm<br>18.5 in  |
| As shipped plus handles                                                     | 280 mm<br>11.0 in | 458 mm<br>18 in    | 501 mm<br>19.7 in  |
| As shipped plus rack-mount flanges                                          | 280 mm<br>11.0 in | 483 mm<br>19 in    | 470 mm<br>18.5 in  |
| As shipped plus handles and rack-mount flanges                              | 280 mm<br>11.0 in | 483 mm<br>19 in    | 501 mm<br>19.70 in |

| <b>Weight</b>   |                          |
|-----------------|--------------------------|
| <b>Net</b>      |                          |
| N5230A          | 24.9 kg (55 lb), nominal |
| <b>Shipping</b> |                          |
| N5230A          | 36.3 kg (80 lb), nominal |

## Measurement Throughput Summary

[Typical Cycle Time for Measurement Completion](#)

[Cycle Time vs IF Bandwidth](#)

[Cycle Time vs Number of Points](#)

[Data Transfer Time](#)

**Table 24.** Typical Cycle Time<sup>a</sup> (ms) for Measurement Completion



| Description                                           | Typical                 |            |            |             |               |
|-------------------------------------------------------|-------------------------|------------|------------|-------------|---------------|
|                                                       | <b>Number of Points</b> |            |            |             |               |
|                                                       | <b>201</b>              | <b>401</b> | <b>801</b> | <b>1601</b> | <b>16,001</b> |
| <b>Start 8 GHz, Stop 18 GHz, 30 kHz IF bandwidth</b>  |                         |            |            |             |               |
| Uncorrected                                           | 97.5                    | 102.7      | 103.8      | 108.2       | 683.9         |
| 2-Port cal                                            | 203.7                   | 213.5      | 218.5      | 234.6       | 1504.3        |
| <b>Start 10 MHz, Stop 10 GHz, 30 kHz IF bandwidth</b> |                         |            |            |             |               |
| Uncorrected                                           | 112.6                   | 120.6      | 124.8      | 138.2       | 738.4         |
| 2-Port cal                                            | 232.8                   | 251.8      | 265.2      | 304.3       | 1623.4        |
| <b>Start 10 MHz, Stop 20 GHz, 30 kHz IF bandwidth</b> |                         |            |            |             |               |
| Uncorrected                                           | 146                     | 199.3      | 210.9      | 217.2       | 753.9         |
| 2-Port cal                                            | 302.3                   | 410.5      | 438.7      | 462.5       | 1660.5        |
| <b>Start 8 GHz, Stop 18 GHz, 50 kHz IF bandwidth</b>  |                         |            |            |             |               |
| Uncorrected                                           | 79.1                    | 81         | 81.7       | 86.6        | 482           |
| 2-Port cal                                            | 164.5                   | 170.3      | 175.3      | 193.5       | 1104.7        |
| <b>Start 10 MHz, Stop 10 GHz, 50 kHz IF bandwidth</b> |                         |            |            |             |               |
| Uncorrected                                           | 96.8                    | 101.7      | 108.8      | 122.2       | 524.6         |
| 2-Port cal                                            | 202.1                   | 215.6      | 236.7      | 276.7       | 1198.8        |
| <b>Start 10 MHz, Stop 20 GHz, 50 kHz IF bandwidth</b> |                         |            |            |             |               |
| Uncorrected                                           | 141.6                   | 163.9      | 170.7      | 179.7       | 546.5         |
| 2-Port cal                                            | 293.6                   | 341        | 360        | 389.5       | 1248.8        |

<sup>a</sup> Includes sweep time, retrace time and band-crossing time. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S<sub>11</sub>) measurement.

**Table 25. (Options 020/025, 120/125, only) Cycle Time vs IF Bandwidth**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 10 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Description | Typical Performance |
|-------------|---------------------|
|-------------|---------------------|

| IF Bandwidth (Hz) | Cycle Time (ms) <sup>a</sup> | Trace Noise (dB rms) |
|-------------------|------------------------------|----------------------|
| 600,000           | 7                            | 0.0035               |
| 360,000           | 7                            | 0.0026               |
| 280,000           | 7                            | 0.0022               |
| 200,000           | 7                            | 0.0021               |
| 150,000           | 7                            | 0.0016               |
| 100,000           | 7                            | 0.0012               |
| 70,000            | 7                            | 0.0011               |
| 50,000            | 9                            | 0.0009               |
| 30,000            | 11                           | 0.0008               |
| 20,000            | 14                           | 0.0006               |
| 15,000            | 17                           | 0.0005               |
| 10,000            | 28                           | 0.0004               |
| 7000              | 37                           | 0.0004               |
| 5000              | 48                           | 0.0003               |
| 3000              | 72                           | 0.0003               |
| 2000              | 102                          | 0.0002               |
| 1500              | 130                          | 0.0001               |
| 1000              | 218                          | 0.0001               |
| 700               | 294                          | 0.0001               |
| 500               | 399                          | 0.0001               |
| 300               | 636                          | 0.0001               |
| 200               | 932                          | 0                    |
| 100               | 1826                         | 0                    |
| 30                | 6004                         | 0                    |

|    |        |   |
|----|--------|---|
| 10 | 17903  | 0 |
| 1  | 178398 | 0 |

a Cycle time includes sweep and retrace time.

**Table 26. (Options 220/225, 420/425, 520/525 only) Cycle Time vs IF Bandwidth**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 10 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Description | Typical                      |                                       |
|-------------|------------------------------|---------------------------------------|
|             | Cycle Time (ms) <sup>a</sup> | Cycle Time (ms)<br>Option 080 enabled |
| 250,000     | 8.9                          | 37.9                                  |
| 200,000     | 9.3                          | 39.3                                  |
| 150,000     | 9.9                          | 40.1                                  |
| 100,000     | 10.5                         | 41.8                                  |
| 70,000      | 11.5                         | 43.6                                  |
| 50,000      | 12.8                         | 45.4                                  |
| 30,000      | 15.4                         | 50                                    |
| 20,000      | 18.3                         | 53.9                                  |
| 15,000      | 21                           | 57.5                                  |
| 10,000      | 27                           | 65.8                                  |
| 7000        | 34                           | 75.4                                  |
| 5000        | 48.5                         | 93                                    |
| 3000        | 72.8                         | 124                                   |
| 2000        | 108.8                        | 169                                   |
| 1500        | 126.8                        | 187.1                                 |

|      |          |
|------|----------|
| 1000 | 272.5    |
| 700  | 357.7    |
| 500  | 460      |
| 300  | 697.7    |
| 200  | 1003.5   |
| 150  | 1307.8   |
| 100  | 1917.6   |
| 30   | 6173.8   |
| 10   | 18214.8  |
| 1    | 181699.2 |

a Cycle time includes sweep and retrace time.

**Table 27. (Options 020/025, 120/125, only) Cycle Time vs Number of Points**

Applies to the Preset condition (correction off) except for the following changes:

- CF = 10 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Description | Typical Performance |                              |
|-------------|---------------------|------------------------------|
|             | Number of Points    | Cycle Time (ms) <sup>a</sup> |
| 30,000      | 3                   | 6.7                          |
|             | 11                  | 7.4                          |
|             | 51                  | 6.9                          |
|             | 101                 | 7.8                          |
|             | 201                 | 11.2                         |
|             | 401                 | 18.3                         |
|             | 801                 | 32.4                         |
|             | 1,601               | 59.4                         |
|             | 6,401               | 224.7                        |
|             | 16,001              | 556.9                        |

|         |        |       |
|---------|--------|-------|
| 100,000 | 3      | 6.7   |
|         | 11     | 6.6   |
|         | 51     | 6.8   |
|         | 101    | 7     |
|         | 201    | 7.5   |
|         | 401    | 9     |
|         | 801    | 13.5  |
|         | 1,601  | 22.9  |
|         | 6,401  | 75.3  |
|         | 16,001 | 180.3 |
| 600,000 | 3      | 6.5   |
|         | 11     | 6.6   |
|         | 51     | 6.8   |
|         | 101    | 6.9   |
|         | 201    | 7.3   |
|         | 401    | 8.1   |
|         | 801    | 9.4   |
|         | 1,601  | 12    |
|         | 6,401  | 27.7  |
|         | 16,001 | 59.3  |

a Cycle time includes sweep and retrace time.

**Table 28. (Options 220/225, 420/425, 520/525 only) Cycle Time vs Number of Points**

Applies to the Preset condition (correction off) except for the following changes:

- CF = 10 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Description       | Typical          |                              |
|-------------------|------------------|------------------------------|
| IF Bandwidth (Hz) | Number of Points | Cycle Time (ms) <sup>a</sup> |
| 30,000            | 3                | 8                            |
|                   | 11               | 8                            |
|                   | 51               | 9.38                         |
|                   | 101              | 11.4                         |
|                   | 201              | 15.5                         |
|                   | 401              | 23.6                         |
|                   | 801              | 39.9                         |
|                   | 1,601            | 71.6                         |
|                   | 6,401            | 265.4                        |
|                   | 16,001           | 650.8                        |
| 50,000            | 3                | 7.7                          |
|                   | 11               | 7.7                          |
|                   | 51               | 8.7                          |
|                   | 101              | 10.1                         |
|                   | 201              | 13                           |
|                   | 401              | 18.6                         |
|                   | 801              | 29.8                         |
|                   | 1,601            | 52.3                         |
|                   | 6,401            | 184.5                        |
|                   | 16,001           | 448.8                        |
| 250,000           | 101              | 8.7                          |
|                   | 201              | 9.05                         |
|                   | 401              | 10.85                        |
|                   | 801              | 14.42                        |
|                   | 1,601            | 21.63                        |
|                   | 6,401            | 61.1                         |
|                   | 16,001           | 147.7                        |

<sup>a</sup> Cycle time includes sweep and retrace time.

**Table 29.** Data Transfer Time (ms)

| Description                                                       | Typical          |     |      |        |
|-------------------------------------------------------------------|------------------|-----|------|--------|
|                                                                   | Number of Points |     |      |        |
|                                                                   | 201              | 401 | 1601 | 16,001 |
| <b>SCPI over GPIB</b><br><b>(program executed on external PC)</b> |                  |     |      |        |
| 32-bit floating point                                             | 7                | 12  | 43   | 435    |
| 64-bit floating point                                             | 12               | 22  | 84   | 856    |
| ASCII                                                             | 64               | 124 | 489  | 5054   |
| <b>SCPI</b><br><b>(program executed in the analyzer)</b>          |                  |     |      |        |
| 32-bit floating point                                             | 1                | 2   | 3    | 30     |
| 64-bit floating point                                             | 2                | 2   | 4    | 40     |
| ASCII                                                             | 29               | 56  | 222  | 2220   |
| <b>COM (program executed in the analyzer)</b>                     |                  |     |      |        |
| 32-bit floating point                                             | <0.4             | 0.4 | 0.5  | 1.9    |
| Variant type                                                      | 0.7              | 1   | 3    | 32     |
| <b>DCOM over LAN</b><br><b>(program executed on external PC)</b>  |                  |     |      |        |
| 32-bit floating point                                             | <0.8             | 1   | 1.5  | 7.1    |
| Variant type                                                      | 1.8              | 2.7 | 8.5  | 80     |

---


**Note:** Specifications for Recall & Sweep Speed are not provided for the N5230A analyzers.

---


### **Tables 30 - 35 Front-panel Jumper Specs (Options 025, 125, 225, 425, 525)**

#### **Test Set Block Diagrams**

N5230A Option 020, or 120, or 220, or 420, or 520 (Standard Test Set and Standard Power Range)

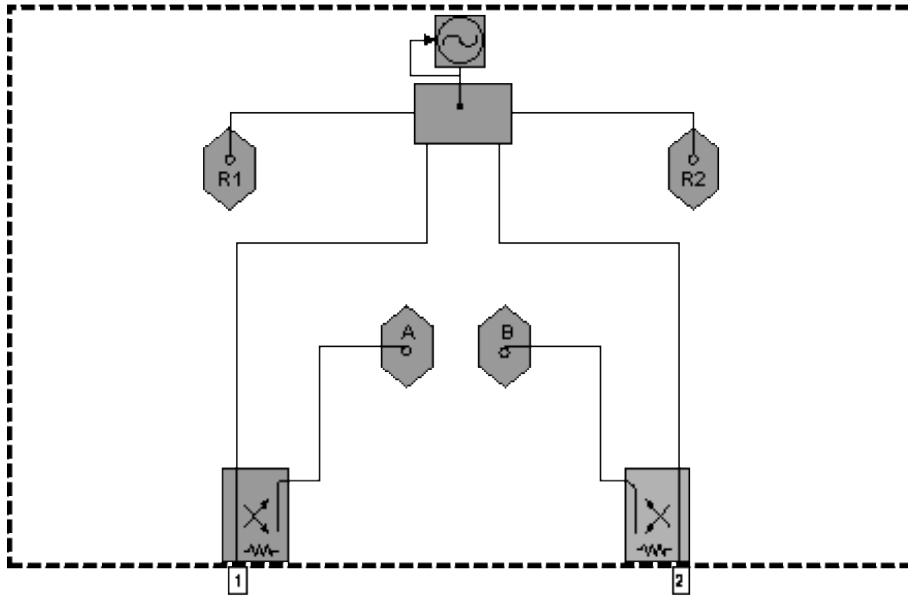

N5230A Option 025, or 125, or 225, or 425, or 525 (Configurable Test Set and Extended Power Range)

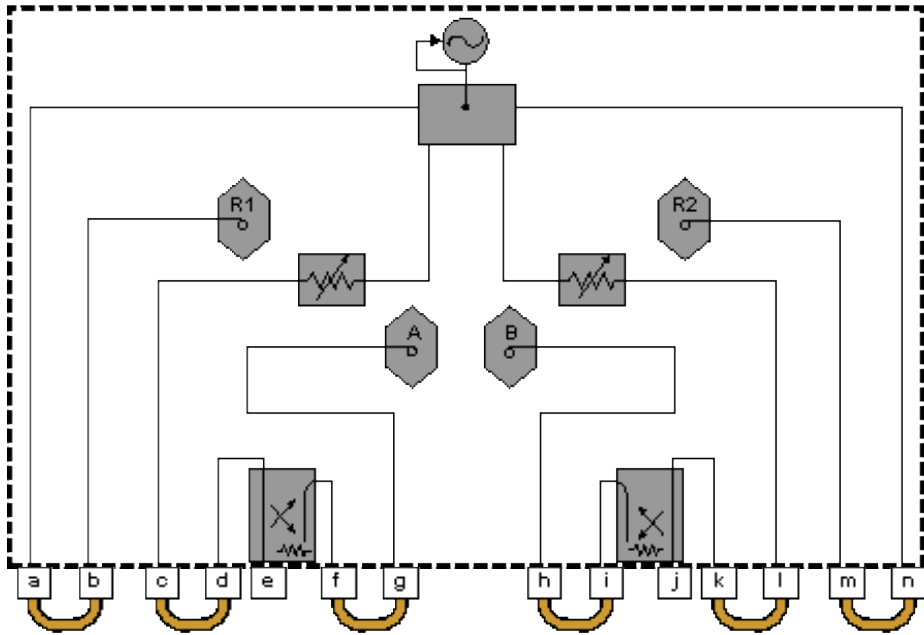



| <b>Item</b> | <b>Description</b> | <b>Item</b> | <b>Description</b> |
|-------------|--------------------|-------------|--------------------|
| <b>a</b>    | SOURCE OUT         | <b>h</b>    | RCVR B IN          |
| <b>b</b>    | RCVR R1 IN         | <b>i</b>    | CPLR ARM           |
| <b>c</b>    | SOURCE OUT         | <b>j</b>    | PORT 2             |
| <b>d</b>    | CPLR THRU          | <b>k</b>    | CPLR THRU          |
| <b>e</b>    | PORT 1             | <b>l</b>    | SOURCE OUT         |
| <b>f</b>    | CPLR ARM           | <b>m</b>    | RCVR R2 IN         |
| <b>g</b>    | RCVR A IN          | <b>n</b>    | SOURCE OUT         |

## Technical Specifications for the N5230A

### Options 240 and 245 (4-Port PNA)

(Rev. 2005-06-01)

---

This is a complete list of the N5230A Options 240, 245 network analyzer technical specifications.

- To optimize viewing of uncertainty curves, click the Maximize button.
  - To view or print the .pdf version of the specifications, visit our web site at <http://www.agilent.com/find/pna>, and search for "N5230A Specifications"
  - This N5230A document provides technical specifications for the 85052B calibration kit and the N4691A ECal module. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the curves for your calibration kit and PNA setup.
- 

#### Definitions

#### Corrected System Performance

##### System Dynamic Range

##### Extended Dynamic Range

##### 3.5mm Connectors

#### Uncorrected System Performance

##### Test Port Output

##### Test Port Input

##### Dynamic Accuracy

##### Group Delay

##### General Information

##### Measurement Throughput Summary

##### Front-panel Jumper Specs (Option 245 only)

##### Option 240 Analyzer Block Diagram

##### Option 245 Analyzer Block Diagram

[See Specs for other PNA models](#)

---

## Definitions

All specifications and characteristics apply over a 25 °C  $\pm$ 5 °C range (unless otherwise stated) and 90 minutes after the instrument has been turned on.

**Specification (spec.):** Warranted performance. Specifications include guardbands to account for the expected statistical performance distribution, measurement uncertainties, and changes in performance due to environmental conditions.

**Characteristic (char.):** A performance parameter that the product is expected to meet before it leaves the factory, but that is not verified in the field and is not covered by the product warranty. A characteristic includes the same guardbands as a specification.

**Typical (typ.):** Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Nominal (nom.):** A general, descriptive term that does not imply a level of performance. It is not covered by the product warranty.

**Calibration:** The process of measuring known standards to characterize a network analyzer's systematic (repeatable) errors.

**Corrected (residual):** Indicates performance after error correction (calibration). It is determined by the quality of calibration standards and how well "known" they are, plus system repeatability, stability, and noise.

**Uncorrected (raw):** Indicates instrument performance without error correction. The uncorrected performance affects the stability of a calibration.

**Standard:** When referring to the analyzer, this includes no options unless noted otherwise.

---

## Corrected System Performance

The specifications in this section apply for measurements made with the N5230A analyzer with the following conditions:

- 10 Hz IF bandwidth
- No averaging applied to data
- Isolation calibration with an averaging factor of 8

### System Dynamic Range

### Extended Dynamic Range

### 3.5mm Connectors

**Table 1.** System Dynamic Range at Test Port <sup>1</sup>

| Description                                                         | Specification (dB) at Test Port | Typical (dB) at Test Port |
|---------------------------------------------------------------------|---------------------------------|---------------------------|
| <b>Standard configuration and standard power range (Option 240)</b> |                                 |                           |
| 300 KHz to 10 MHz <sup>2</sup>                                      | --                              | 111 dB                    |
| 10 MHz to 4 GHz <sup>2</sup>                                        | 120 dB                          | 128 dB                    |
| 4 GHz to 6 GHz                                                      | 118 dB                          | 129 dB                    |
| 6 GHz to 10.5 GHz                                                   | 115 dB                          | 127 dB                    |
| 10.5 GHz to 15 GHz                                                  | 107 dB                          | 119 dB                    |
| 15 GHz to 20 GHz                                                    | 103 dB                          | 116 dB                    |
| <b>Configurable test set and extended power range (Option 245)</b>  |                                 |                           |
| 300 KHz to 10 MHz <sup>2</sup>                                      | --                              | 111 dB                    |
| 10 MHz to 4 GHz <sup>2</sup>                                        | 120 dB                          | 128 dB                    |
| 4 GHz to 6 GHz                                                      | 118 dB                          | 128 dB                    |
| 6 GHz to 10.5 GHz                                                   | 113 dB                          | 125 dB                    |
| 10.5 GHz to 15 GHz                                                  | 105 dB                          | 117 dB                    |
| 15 GHz to 20 GHz                                                    | 98 dB                           | 115 dB                    |

1 The system dynamic range is calculated as the difference between the noise floor and the specified source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account.

2 May be degraded by 10 dB at particular frequencies (multiples of 5 MHz) below 500 MHz due to spurious receiver residuals. Methods are available to regain the full dynamic range.

**Table 2.** Extended Dynamic Range at Direct Receiver Access Input<sup>1</sup>

| <b>Configurable test set and extended power range (Option 245)</b> |                           |                     |
|--------------------------------------------------------------------|---------------------------|---------------------|
|                                                                    | <b>Specification (dB)</b> | <b>Typical (dB)</b> |
| 300 KHz to 10 MHz <sup>2</sup>                                     | --                        | 127 dB              |
| 10 MHz to 4 GHz <sup>2</sup>                                       | 136 dB                    | --                  |
| 4 GHz to 6 GHz                                                     | 134 dB                    | --                  |
| 6 GHz to 10.5 GHz                                                  | 129 dB                    | --                  |
| 10.5 GHz to 15 GHz                                                 | 121 dB                    | --                  |
| 15 GHz to 20 GHz                                                   | 114 dB                    | --                  |

1 The direct receiver access input extended dynamic range is calculated as the difference between the direct receiver access input noise floor and the source maximum output power. The effective dynamic range must take measurement uncertainties and interfering signals into account. This set-up should only be used when the receiver input will never exceed its compression or damage level. When the analyzer is in segment sweep mode, it can have predefined frequency segments which will output a higher power level when the extended dynamic range is required (i.e. devices with high insertion loss), and reduced power when receiver compression or damage may occur (i.e. devices with low insertion loss). The extended range is only available in one-path transmission measurements.

2 May be degraded by 10 dB at particular frequencies (multiples of 5 MHz) below 500 MHz due to spurious receiver residuals. Methods are available to regain the full dynamic range.

Corrected System Performance with 3.5mm Connectors (Tables 3 - 6)

Receiver Dynamic Range technical specifications are not provided in this N5230A specs document.

**Table 7. Uncorrected System Performance<sup>1</sup>**

| <b>Description</b>  | <b>Specification</b>    | <b>Typical</b>          |
|---------------------|-------------------------|-------------------------|
|                     | <b>Options 240, 245</b> | <b>Options 240, 245</b> |
| <b>Directivity</b>  |                         |                         |
| 300 KHz to 10 MHz   | --                      | -23 dB                  |
| 10 MHz to 1 GHz     | -28 dB                  | --                      |
| 1 GHz to 3 GHz      | -25 dB                  | --                      |
| 3 GHz to 5 GHz      | -20 dB                  | --                      |
| 5 GHz to 11.5 GHz   | -17 dB                  | --                      |
| 11.5 GHz to 20 GHz  | -15 dB                  | --                      |
| <b>Source Match</b> |                         |                         |
| 300 KHz to 10 MHz   | --                      | -8 dB                   |
| 10 MHz to 1 GHz     | -12 dB                  | --                      |

|                              |         |         |
|------------------------------|---------|---------|
| 1 GHz to 3 GHz               | -12 dB  | --      |
| 3 GHz to 5 GHz               | -12 dB  | --      |
| 5 GHz to 10.5 GHz            | -12 dB  | --      |
| 10.5 GHz to 11.5 GHz         | -10 dB  | --      |
| 11.5 GHz to 20 GHz           | -8 dB   | --      |
| <b>Load Match</b>            |         |         |
| 300 KHz to 10 MHz            | --      | -9 dB   |
| 10 MHz to 1 GHz              | -20 dB  | --      |
| 1 GHz to 3 GHz               | -20 dB  | --      |
| 3 GHz to 5 GHz               | -18 dB  | --      |
| 5 GHz to 11.5 GHz            | -12 dB  | --      |
| 11.5 GHz to 16 GHz           | -7 dB   | --      |
| 16 GHz to 20 GHz             | -7.5 dB | --      |
| <b>Crosstalk<sup>2</sup></b> |         |         |
| 300 KHz to 5 MHz             | --      | -70 dB  |
| 5 MHz-10 MHz                 | --      | -100 dB |
| 10 MHz to 45 MHz             | --      | -110 dB |
| 45 MHz to 4 GHz              | --      | -122 dB |
| 4 GHz to 6 GHz               | --      | -123 dB |
| 6 GHz to 10.5 GHz            | --      | -120 dB |
| 10.5 GHz to 15 GHz           | --      | -115 dB |
| 15 GHz to 20 GHz             | --      | -110 dB |

1 Specifications apply over environmental temperature of 25 °C ±5 °C, with less than 1°C variation from the calibration temperature.

2 Measurement conditions: normalized to a thru, measured with two shorts, 10 Hz IF bandwidth, averaging factor of 8, alternate mode, source power set to the lesser of the maximum power out or the maximum receiver power.

**Table 8.** Test Port Output<sup>1</sup>

| Description            | Specification |         | Typical |         |
|------------------------|---------------|---------|---------|---------|
|                        | Opt 240       | Opt 245 | Opt 240 | Opt 245 |
| <b>Frequency Range</b> |               |         |         |         |

|                                         |                   |                      |                                                                 |                |
|-----------------------------------------|-------------------|----------------------|-----------------------------------------------------------------|----------------|
|                                         | 300 KHz to 20 GHz |                      | --                                                              |                |
| <b>Nominal Power</b>                    |                   |                      |                                                                 |                |
|                                         | -5 dBm            | -8 dBm               | Preset power; attenuator switch point 10 dB below nominal power |                |
| <b>Frequency Resolution</b>             |                   |                      |                                                                 |                |
|                                         | 1 Hz              |                      | --                                                              |                |
| <b>CW Accuracy</b>                      |                   |                      |                                                                 |                |
|                                         | +/-1 ppm          |                      | --                                                              |                |
| <b>Frequency Stability</b>              |                   |                      |                                                                 |                |
|                                         | --                |                      | +/-0.05 ppm. -10° to 70° C<br>+/-0.1 ppm/yr maximum             |                |
| <b>Description</b>                      |                   | <b>Specification</b> |                                                                 | <b>Typical</b> |
|                                         | <b>Opt 240</b>    | <b>Opt 245</b>       | <b>Opt 240</b>                                                  | <b>Opt 245</b> |
| <b>Power Level Accuracy</b>             |                   |                      |                                                                 |                |
| Variation from nominal power in range 0 |                   |                      |                                                                 |                |
| 300 KHz to 10 MHz                       | --                | --                   | +/-1.0 dB                                                       | +/-1.0 dB      |
| 10 MHz to 2 GHz                         | +/-1.0 dB         | +/-1.0 dB            | --                                                              | --             |
| 2 GHz to 10.5 GHz                       | +/-1.5 dB         | +/-1.5 dB            | --                                                              | --             |
| 10.5 GHz to 20 GHz                      | +/-2.5 dB         | +/-2.5 dB            | --                                                              | --             |
| <b>Max Leveled Power</b>                |                   |                      |                                                                 |                |
| 300 KHz to 10 MHz                       | --                | --                   | +8 dBm                                                          | +8 dBm         |
| 10 MHz to 4 GHz                         | +8 dBm            | +8 dBm               | +12 dBm                                                         | +11 dBm        |
| 4 GHz to 6 GHz                          | +6 dBm            | +6 dBm               | +10 dBm                                                         | +9 dBm         |
| 6 GHz to 10.5 GHz                       | +3 dBm            | +1 dBm               | +8 dBm                                                          | +6 dBm         |
| 10.5 GHz to 15 GHz                      | 0 dBm             | -2 dBm               | +5 dBm                                                          | +3 dBm         |
| 15 GHz to 20 GHz                        | -3 dBm            | -8 dBm               | +2 dBm                                                          | -1 dBm         |
| <b>Power Level Linearity</b>            |                   |                      |                                                                 |                |

|                                                                                                               |                      |                |                |                |
|---------------------------------------------------------------------------------------------------------------|----------------------|----------------|----------------|----------------|
| Specified on Port 1 only. Ports 2, 3, 4 performance is Typical. Test reference is at the nominal power level. |                      |                |                |                |
| 300 KHz to 10 MHz                                                                                             | --                   | --             | +/-2.0 dB      | +/-2.0 dB      |
| 10 MHz to 1 GHz                                                                                               | +/-2.0 dB            | +/-2.0 dB      | --             | --             |
| 1 GHz to 20 GHz                                                                                               | +/-1.5 dB            | +/-1.5 dB      | --             | --             |
| <b>Power Sweep Range (ALC)</b>                                                                                |                      |                |                |                |
| ALC range starts at maximum leveled power and decreases by the dB amount specified here.                      |                      |                |                |                |
| 300 KHz to 10 MHz                                                                                             | --                   | --             | 35 dB          | 35 dB          |
| 10 MHz to 4 GHz                                                                                               | 33 dB                | 33 dB          | --             | --             |
| 4 GHz to 6 GHz                                                                                                | 31 dB                | 31 dB          | --             | --             |
| 6 GHz to 10.5 GHz                                                                                             | 28 dB                | 26 dB          | --             | --             |
| 10.5 GHz to 15 GHz                                                                                            | 25 dB                | 23 dB          | --             | --             |
| 15 GHz to 20 GHz                                                                                              | 22 dB                | 17 dB          | --             | --             |
| <b>Description</b>                                                                                            | <b>Specification</b> |                | <b>Typical</b> |                |
|                                                                                                               | <b>Opt 240</b>       | <b>Opt 245</b> | <b>Opt 240</b> | <b>Opt 245</b> |
| <b>Power Resolution</b>                                                                                       |                      |                |                |                |
|                                                                                                               | 0.01 dB              | 0.01 dB        | --             | --             |
| <b>Power Range</b>                                                                                            |                      |                |                |                |
| 300 KHz to 10 MHz                                                                                             | --                   | --             | -27 to +8 dBm  | -87 to +8 dBm  |
| 10 MHz to 45MHz                                                                                               | --                   | --             | -27 to +12 dBm | -87 to +11 dBm |
| 45 MHz to 4 GHz                                                                                               | --                   | --             | -27 to +12 dBm | -87 to +11 dBm |
| 4 GHz to 6 GHz                                                                                                | --                   | --             | -27 to +10 dBm | -87 to +9 dBm  |
| 6 GHz to 10.5 GHz                                                                                             | --                   | --             | -27 to +8 dBm  | -87 to +6 dBm  |
| 10.5 GHz to 15 GHz                                                                                            | --                   | --             | -27 to +5 dBm  | -87 to +3 dBm  |
| 15 GHz to 20 GHz                                                                                              | --                   | --             | -27 to +2 dBm  | -87 to -1 dBm  |
| <b>Power Settings</b>                                                                                         |                      |                |                |                |
| Minimum Power Setting                                                                                         | --                   | --             | -30 dBm        | -90 dBm        |
| Maximum Power Setting                                                                                         | --                   | --             | +20 dBm        | +20 dBm        |



| Harmonics (2nd or 3rd) at Maximum Output Power  |    |    |                                      |
|-------------------------------------------------|----|----|--------------------------------------|
| In-band Source Harmonics                        |    |    |                                      |
| 300 KHz to 10 MHz                               | -- | -- | -17 dBc                              |
| 10 MHz to 1 GHz                                 | -- | -- | -17 dBc                              |
| 1 GHz to 20 GHz                                 | -- | -- | -20 dBc                              |
| Non-Harmonic Spurious (at Nominal Output Power) |    |    |                                      |
| 300 KHz to 20 GHz                               | -- | -- | -50 dBc for offset frequency > 1 KHz |

1 Performance specified on Port 1 only; Ports 2, 3, and 4 performance is typical. Test reference is at the nominal power level.

**Table 8. Test Port Output (Continued)**

| Phase Noise (Nominal power at test port) | Typical Performance |                |              |
|------------------------------------------|---------------------|----------------|--------------|
|                                          | 10 kHz Offset       | 100 kHz Offset | 1 MHz Offset |
| 300 KHz to 10 MHz                        | -86 dBc/Hz          | -86 dBc/Hz     | -95 dBc/Hz   |
| 10 MHz to 1.5 GHz                        | -86 dBc/Hz          | -91 dBc/Hz     | -95 dBc/Hz   |
| 1.5 GHz to 3.125 GHz                     | -83 dBc/Hz          | -91 dBc/Hz     | -95 dBc/Hz   |
| 3.125 GHz to 6.25 GHz                    | -77 dBc/Hz          | -85 dBc/Hz     | -89 dBc/Hz   |
| 6.25 GHz to 12.5 GHz                     | -71 dBc/Hz          | -79 dBc/Hz     | -83 dBc/Hz   |
| 12.5 GHz to 20 GHz                       | -65 dBc/Hz          | -73 dBc/Hz     | -77 dBc/Hz   |

**Table 9. Test Port Input**

| Description                                                                                                | Specification    | Typical          |
|------------------------------------------------------------------------------------------------------------|------------------|------------------|
|                                                                                                            | Options 240, 245 | Options 240, 245 |
| Test Port Noise Floor                                                                                      |                  |                  |
| Total average (rms) noise power calculated as the mean value of a linear magnitude trace expressed in dBm. |                  |                  |
| 10 Hz IF Bandwidth                                                                                         |                  |                  |
| 300 KHz to 10 MHz                                                                                          | --               | <-103 dBm        |
| 10 MHz to 500 MHz                                                                                          | <-112 dBm        | <-116 dBm        |
| 500 MHz to 4 GHz                                                                                           | <-112 dBm        | <-120 dBm        |

|                                                                                                            |           |           |
|------------------------------------------------------------------------------------------------------------|-----------|-----------|
| 4 GHz to 10.5 GHz                                                                                          | <-112 dBm | <-119 dBm |
| 10.5 GHz to 15 GHz                                                                                         | <-107 dBm | <-114 dBm |
| 15 GHz to 20 GHz                                                                                           | <-106 dBm | <-114 dBm |
| <b>1 KHz IF Bandwidth</b>                                                                                  |           |           |
| 300 KHz to 10 MHz                                                                                          | --        | <-83 dBm  |
| 10 MHz to 500 MHz                                                                                          | <-92 dBm  | <-96 dBm  |
| 500 MHz to 4 GHz                                                                                           | <-92 dBm  | <-100 dBm |
| 4 GHz to 10.5 GHz                                                                                          | <-92 dBm  | <-99 dBm  |
| 10.5 GHz to 15 GHz                                                                                         | <-87 dBm  | <-94 dBm  |
| 15 GHz to 20 GHz                                                                                           | <-86 dBm  | <-94 dBm  |
| <b>Direct Receiver Access Input Noise Floor (Option 245 Only)</b>                                          |           |           |
| Total average (rms) noise power calculated as the mean value of a linear magnitude trace expressed in dBm. |           |           |
| <b>10 Hz IF Bandwidth</b>                                                                                  |           |           |
| 300 KHz to 10 MHz                                                                                          | --        | <-119 dBm |
| 10 MHz to 500 MHz                                                                                          | <-128 dBm | <-132 dBm |
| 500 MHz to 4 GHz                                                                                           | <-128 dBm | <-136 dBm |
| 4 GHz to 10.5 GHz                                                                                          | <-128 dBm | <-135 dBm |
| 10.5 GHz to 15 GHz                                                                                         | <-123 dBm | <-130 dBm |
| 15 GHz to 20 GHz                                                                                           | <-122 dBm | <-130 dBm |
| <b>1 KHz IF Bandwidth</b>                                                                                  |           |           |
| 300 KHz to 10 MHz                                                                                          | --        | <-99 dBm  |
| 10 MHz to 500 MHz                                                                                          | <-108 dBm | <-112 dBm |
| 500 MHz to 4 GHz                                                                                           | <-108 dBm | <-116 dBm |
| 4 GHz to 10.5 GHz                                                                                          | <-108 dBm | <-115 dBm |
| 10.5 GHz to 15 GHz                                                                                         | <-103 dBm | <-110 dBm |
| 15 GHz to 20 GHz                                                                                           | <-102 dBm | <-110 dBm |

| Description                                          | Specification    |                  | Typical          |                  |
|------------------------------------------------------|------------------|------------------|------------------|------------------|
|                                                      | Options 240, 245 |                  | Options 240, 245 |                  |
| <b>Compression Level (at +8 dBm except as noted)</b> |                  |                  |                  |                  |
|                                                      | Power            | Com-<br>pression | Power            | Com-<br>pression |
| 300 KHz to 10 MHz                                    | --               | --               | +5 dBm           | 0.10 dB          |
| 10 MHz to 50 MHz                                     | +8 dBm           | 0.35 dB          | --               | --               |
| 50 MHz to 1 GHz                                      | +8 dBm           | 0.35 dB          | --               | --               |
| 1 GHz to 8 GHz                                       | +8 dBm           | 0.25 dB          | --               | --               |
| 8 GHz to 12.5 GHz                                    | +8 dBm           | 0.30 dB          | --               | --               |
| 12.5 GHz to 20 GHz                                   | +8 dBm           | 0.55 dB          | --               | --               |
| <b>Test Port Compression - 0.1 dB</b>                |                  |                  |                  |                  |
| 300 KHz to 10 MHz                                    | --               | --               | +5 dBm           | --               |
| 10 MHz to 1 GHz                                      | --               | --               | +9 dBm           | --               |
| 1 GHz to 12.5 GHz                                    | --               | --               | +10 dBm          | --               |
| 12.5 GHz to 20 GHz                                   | --               | --               | +9 dBm           | --               |

| <b>Table 9. Test Port Input (Continued)</b>      |               |             |             |             |
|--------------------------------------------------|---------------|-------------|-------------|-------------|
| Description                                      | Specification |             | Typical     |             |
|                                                  | Option 240    | Option 245  | Option 240  | Option 245  |
| <b>Trace Noise Magnitude</b>                     |               |             |             |             |
| Ratioed measurement, nominal power at test port. |               |             |             |             |
| <b>100 KHz IF bandwidth</b>                      |               |             |             |             |
| 300 KHz to 10 MHz                                | --            | --          | .015 dB rms | .030 dB rms |
| 10 MHz to 10.5 GHz                               | .006 dB rms   | .008 dB rms | .004 dB rms | .005 dB rms |
| 10.5 GHz to 20 GHz                               | .010 dB rms   | .014 dB rms | .007 dB rms | .009 dB rms |
| <b>600 KHz IF bandwidth</b>                      |               |             |             |             |

|                                                  |              |              |               |               |
|--------------------------------------------------|--------------|--------------|---------------|---------------|
| 300 KHz to 10 MHz                                | --           | --           | .015 dB rms   | .030 dB rms   |
| 10 MHz to 10.5 GHz                               | --           | --           | .013 dB rms   | .015 dB rms   |
| 10.5 GHz to 20 GHz                               | --           | --           | .017 dB rms   | .023 dB rms   |
| <b>100 KHz IF bandwidth</b>                      |              |              |               |               |
| Measured at Maximum Specified Power              |              |              |               |               |
| 300 KHz to 10 MHz                                | --           | --           | .005 dB rms   | .010 dB rms   |
| 10 MHz to 2 GHz                                  | --           | --           | .001 dB rms   | .003 dB rms   |
| 2 GHz to 10.5 GHz                                | --           | --           | .002 dB rms   | .003 dB rms   |
| 10.5 GHz to 20 GHz                               | --           | --           | .006 dB rms   | .009 dB rms   |
| <b>Trace Noise Phase</b>                         |              |              |               |               |
| Ratioed measurement, nominal power at test port. |              |              |               |               |
| <b>100 KHz IF bandwidth</b>                      |              |              |               |               |
| 300 KHz to 10 MHz                                | --           | --           | 0.110 deg rms | 0.180 deg rms |
| 10 MHz to 10.5 GHz                               | 0.05 deg rms | 0.07 deg rms | 0.025 deg rms | 0.035 deg rms |
| 10.5 GHz to 20 GHz                               | 0.08 deg rms | 0.10 deg rms | 0.050 deg rms | 0.060 deg rms |
| <b>600 KHz IF bandwidth</b>                      |              |              |               |               |
| 300 KHz to 10 MHz                                | --           | --           | 0.110 deg rms | 0.180 deg rms |
| 10 MHz to 10.5 GHz                               | --           | --           | 0.080 deg rms | 0.100 deg rms |
| 10.5 GHz to 20 GHz                               | --           | --           | 0.120 deg rms | 0.160 deg rms |
| <b>100 KHz IF bandwidth</b>                      |              |              |               |               |
| Measured at Maximum Specified Power              |              |              |               |               |
| 300 KHz to 10 MHz                                | --           | --           | 0.040 deg rms | 0.050 deg rms |
| 10 MHz to 2 GHz                                  | --           | --           | 0.007 deg rms | 0.012 deg rms |
| 2 GHz to 10.5 GHz                                | --           | --           | 0.012 deg rms | 0.015 deg rms |
| 10.5 GHz to 20 GHz                               | --           | --           | 0.040 deg rms | 0.060 deg rms |
| <b>Reference Level Magnitude</b>                 |              |              |               |               |
| Range                                            | +/-200 dB    | +/-200 dB    | --            | --            |

|                                                                    |         |         |                |    |
|--------------------------------------------------------------------|---------|---------|----------------|----|
| Resolution                                                         | 0.001dB | 0.001dB | --             | -- |
| <b>Reference Level Phase</b>                                       |         |         |                |    |
| Range                                                              | +/-500° | +/-500° | --             | -- |
| Resolution                                                         | 0.01°   | 0.01°   | --             | -- |
| <b>Stability Magnitude</b>                                         |         |         |                |    |
| Stability is defined as a ratio measurement made at the test port. |         |         |                |    |
| 300 KHz to 10 MHz                                                  | --      | --      | +/-0.015 dB/°C |    |
| 10 MHz to 2 GHz                                                    | --      | --      | +/-0.010 dB/°C |    |
| 2 GHz to 4 GHz                                                     | --      | --      | +/-0.015 dB/°C |    |
| 4 GHz to 16 GHz                                                    | --      | --      | +/-0.020 dB/°C |    |
| 16 GHz to 19 GHz                                                   | --      | --      | +/-0.025 dB/°C |    |
| 19 GHz to 20 GHz                                                   | --      | --      | +/-0.030 dB/°C |    |
| <b>Stability Phase</b>                                             |         |         |                |    |
| Stability is defined as a ratio measurement made at the test port. |         |         |                |    |
| 300 KHz to 10 MHz                                                  | --      | --      | +/-0.360°/°C   |    |
| 10 MHz to 45 MHz                                                   | --      | --      | +/-0.020°/°C   |    |
| 45 MHz to 500 MHz                                                  | --      | --      | +/-0.030°/°C   |    |
| 500 MHz to 2 GHz                                                   | --      | --      | +/-0.050°/°C   |    |
| 2 GHz to 4 GHz                                                     | --      | --      | +/-0.100°/°C   |    |
| 4 GHz to 8 GHz                                                     | --      | --      | +/-0.150°/°C   |    |
| 8 GHz to 16 GHz                                                    | --      | --      | +/-0.300°/°C   |    |
| 16 GHz to 20 GHz                                                   | --      | --      | +/-0.350°/°C   |    |

**Table 9. Test Port Input (Continued)**


| Damage Input Level      | Typical Performance  |                      |
|-------------------------|----------------------|----------------------|
|                         | Opt 240              | Opt 245              |
| Test Port 1,2,3, and 4  | +27 dBm or +/-16 VDC | +27 dBm or +/-16 VDC |
| Receivers R,A,B,C,D     | --                   | +15 dBm or +/-16 VDC |
| Source out (reference)  | --                   | +27 dBm or +/-16 VDC |
| Source out (test ports) | --                   | +27 dBm or +/-16 VDC |
| Coupler Thru            | --                   | +27 dBm or +/-16 VDC |
| Coupler Arm             | --                   | +15 dBm or +/-0 VDC  |

**Table 10. Dynamic Accuracy (Specificationa)**


Accuracy of the test port input power reading relative to the reference input power level.

**Dynamic Accuracy, 0.045 GHz**

**Magnitude**

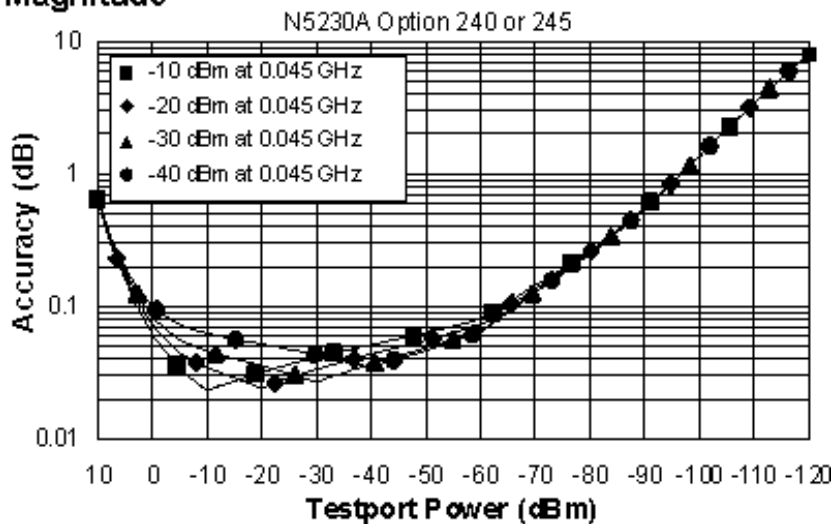


### Phase

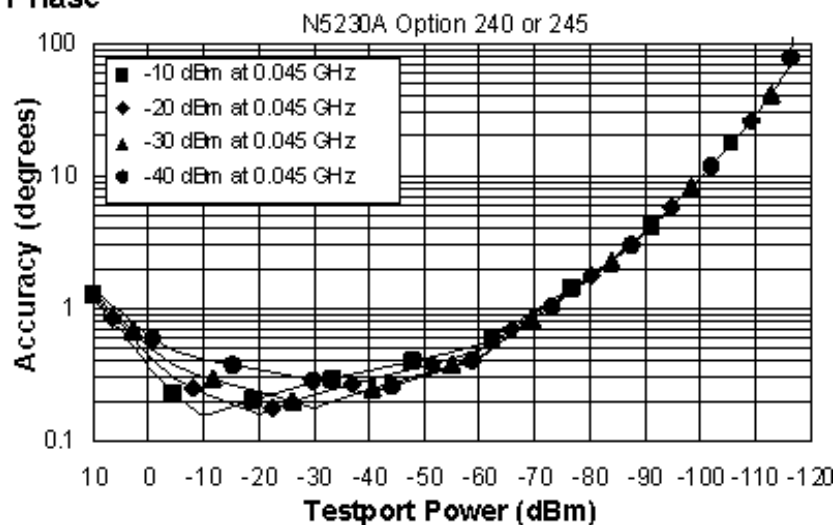


### Dynamic Accuracy, 0.500 GHz

### Magnitude

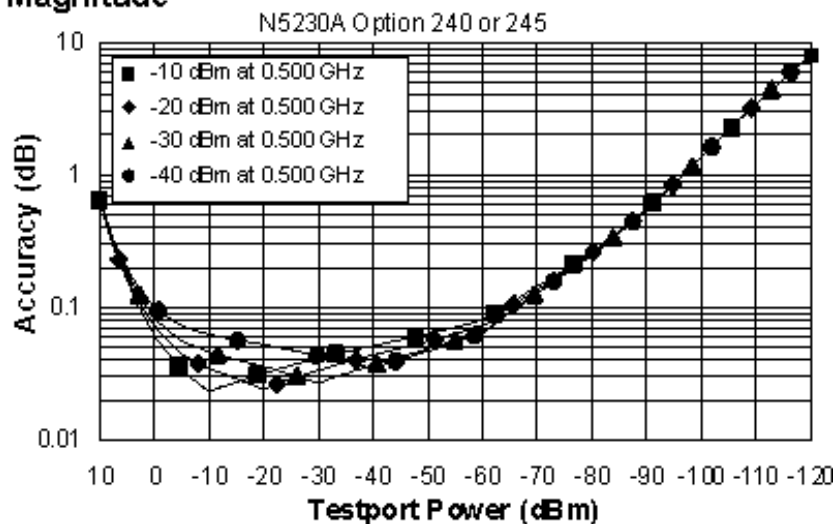


### Phase

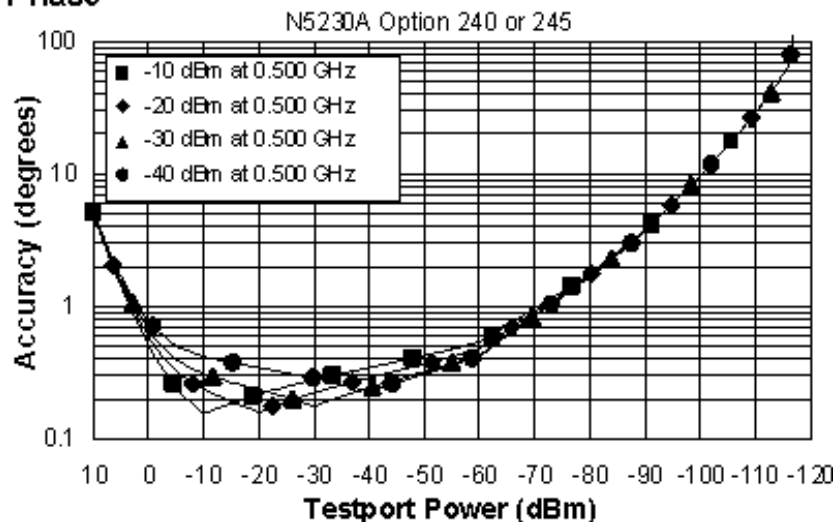


## Dynamic Accuracy, 1- 2 GHz

### Magnitude

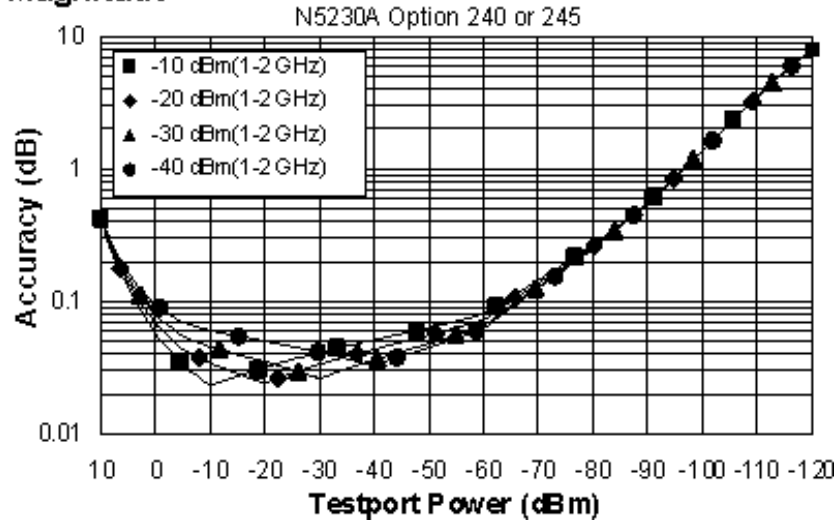

### Phase

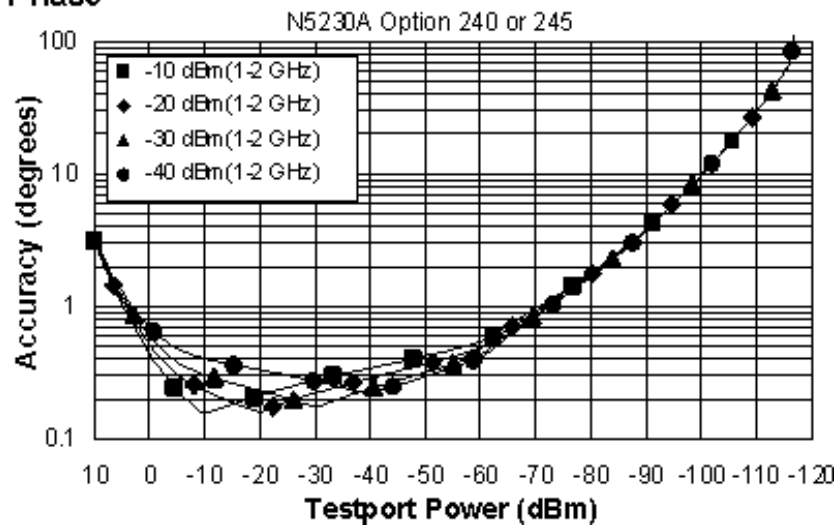


## Dynamic Accuracy, 2 - 12.5 GHz




## Magnitude

N5230 Option 240 or 245

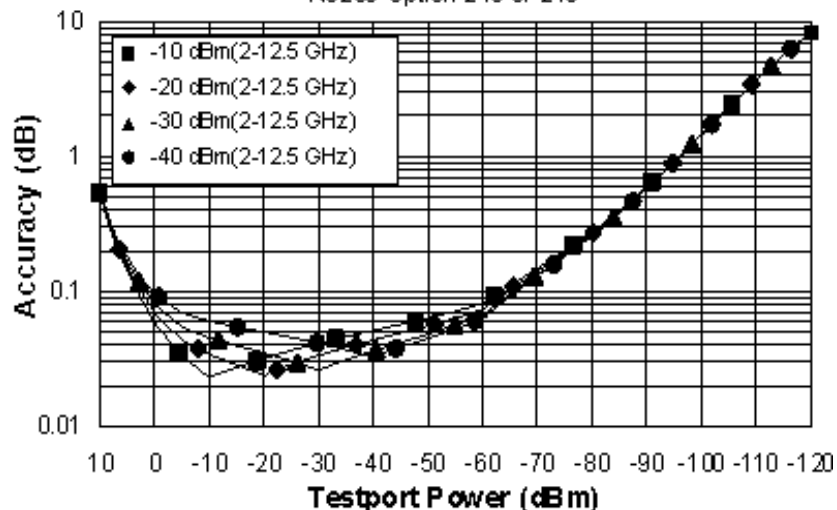

## Phase


N5230 Option 240 or 245

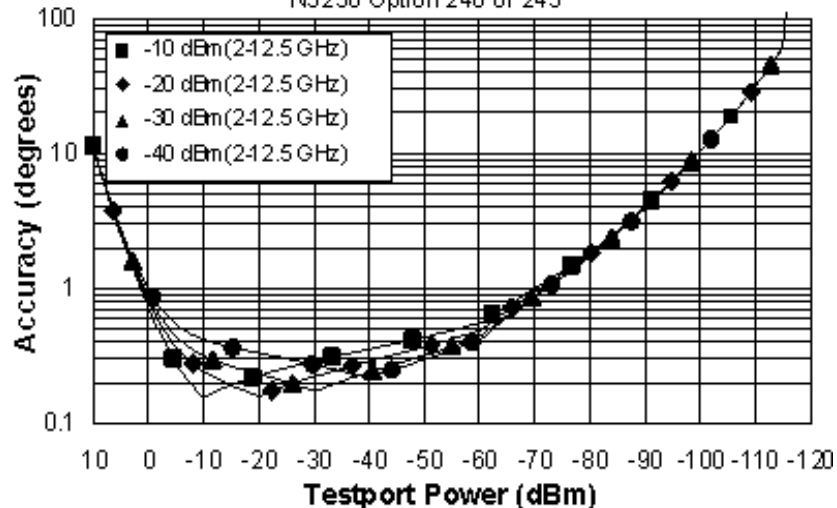


## Dynamic Accuracy, 12.5 - 20 GHz

## Magnitude

N5230A Option 240 or 245

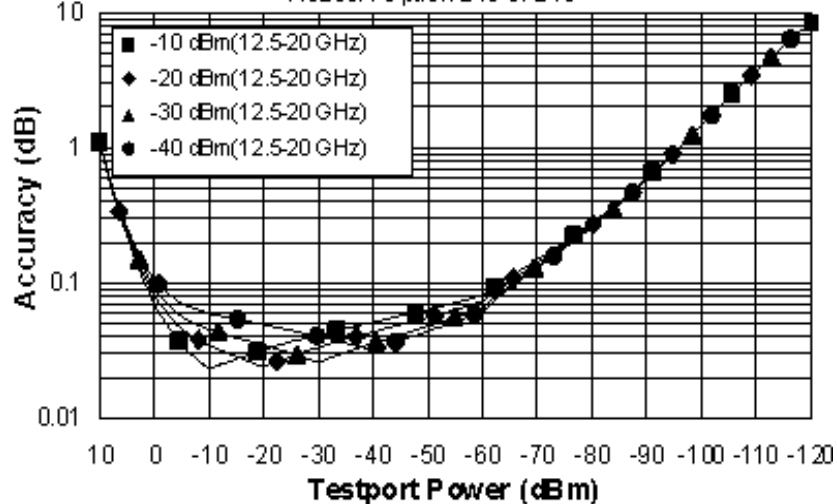

## Phase

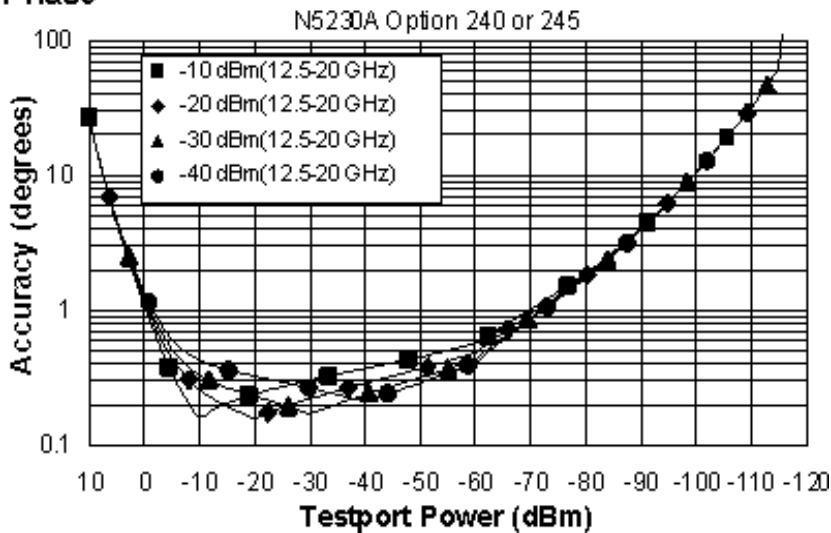

a Dynamic accuracy is verified with the following measurements:

- compression over frequency
- IF linearity at a single frequency of 1.195 GHz using a reference level of -20 dBm for an input power range of 0 to -110 dBm.


**Table 11. Test Port Input (Group Delay)<sup>a</sup>**

| Description           | Supplemental Information (typ.)                                                      |
|-----------------------|--------------------------------------------------------------------------------------|
| Aperture (selectable) | (frequency span)/(number of points -1)                                               |
| Maximum Aperture      | 20% of frequency span                                                                |
| Range                 | 0.5 x (1/minimum aperture)                                                           |
| Maximum Delay         | Limited to measuring no more than 180° of phase change within the minimum aperture.) |
| Accuracy              | See graph below. Char.                                                               |

The following graph shows characteristic group delay accuracy with full 2-port calibration and a 10 Hz IF bandwidth. Insertion loss is assumed to be < 2 dB and electrical length to be ten meters.

For any  $S_{ij}$  Group Delay measurement,  $S_{ii} = 0$ ,  $S_{ij} = 1$ ,  $S_{ji} = 0$ ,  $S_{kl} = 0$  for all  $kl \neq ij$

### Group Delay (Typical)

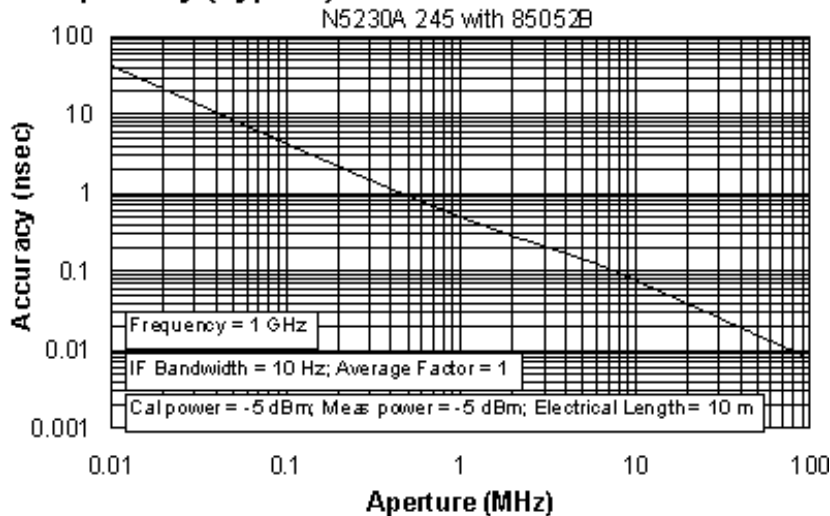

In general, the following formula can be used to determine the accuracy, in seconds, of specific group delay measurement:

$$\pm \text{Phase Accuracy (deg)} / [360 \times \text{Aperture (Hz)}]$$

Depending on the aperture and device length, the phase accuracy used is either incremental phase accuracy or worst case phase accuracy.

a Group delay is computed by measuring the phase change within a specified frequency step (determined by the frequency span and the number of points per sweep).

## General Information

### Miscellaneous Information

#### Front Panel

#### Rear Panel

### Environment and Dimensions

**Table 12.** Miscellaneous Information

| Description               | Supplemental Information    |
|---------------------------|-----------------------------|
| System IF Bandwidth Range | 1 Hz to 600 kHz, nominal    |
| CPU                       | Intel® 500 MHz Pentium® III |

**Table 13.** Front Panel Information

| Description               | Supplemental Information                                                                        |
|---------------------------|-------------------------------------------------------------------------------------------------|
| <b>RF Connectors</b>      |                                                                                                 |
| Type                      | Option 240 or 245: 3.5 mm (male), 50 ohm, (nominal)                                             |
| Center Pin Recession      | 0.002 in. (characteristic)                                                                      |
| <b>Display</b>            |                                                                                                 |
| Size                      | 21.3 cm (8.4 in) diagonal color active matrix LCD; 640 (horizontal) X 480 (vertical) resolution |
| Refresh Rate              | Vertical 59.83 Hz; Horizontal 31.41 kHz                                                         |
| <b>Display Range</b>      |                                                                                                 |
| Magnitude                 | ±500 dB (at 20 dB/div), max                                                                     |
| Phase                     | ±500°, max                                                                                      |
| Polar                     | 10 pUnits, min<br>1000 Units, max                                                               |
| <b>Display Resolution</b> |                                                                                                 |
| Magnitude                 | 0.001 dB/div, min                                                                               |

|                          |                            |
|--------------------------|----------------------------|
| Phase                    | 0.01°/div, min             |
| <b>Marker Resolution</b> |                            |
| Magnitude                | 0.001 dB, min              |
| Phase                    | 0.01°, min                 |
| Polar                    | 0.01 mUnit, min; 0.01°,min |

**Table 14. Rear Panel Information**

| Description                 | Supplemental Information                                                                                                                                                                                           |
|-----------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>10 MHz Reference In</b>  |                                                                                                                                                                                                                    |
| Connector                   | BNC, female                                                                                                                                                                                                        |
| Input Frequency             | 10 MHz ± 10 ppm, Typical                                                                                                                                                                                           |
| Input Level                 | -15 dBm to +20 dBm, Typical                                                                                                                                                                                        |
| Input Impedance             | 200 Ω, nom.                                                                                                                                                                                                        |
| <b>10 MHz Reference Out</b> |                                                                                                                                                                                                                    |
| Connector                   | BNC, female                                                                                                                                                                                                        |
| Output Frequency            | 10 MHz ± 1 ppm, Typical                                                                                                                                                                                            |
| Signal Type                 | Sine Wave, Typical                                                                                                                                                                                                 |
| Output Level                | +10 dBm ± 4 dB into 50 Ω, Typical                                                                                                                                                                                  |
| Output Impedance            | 50 Ω, nominal                                                                                                                                                                                                      |
| Harmonics                   | <-40 dBc, Typical                                                                                                                                                                                                  |
| <b>VGA Video Output</b>     |                                                                                                                                                                                                                    |
| Connector                   | 15-pin mini D-Sub; Drives VGA compatible monitors                                                                                                                                                                  |
| <b>Devices Supported</b>    | <b>Resolutions:</b>                                                                                                                                                                                                |
| Flat Panel (TFT)            | 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                                   |
| Flat Panel (DSTN)           | 800 X 600, 640 X 480                                                                                                                                                                                               |
| CRT Monitor                 | 1280 X 1024, 1024 X 768, 800 X 600, 640 X 480                                                                                                                                                                      |
|                             | Simultaneous operation of the internal and external displays is allowed, but with 640 X 480 resolution only. If you change resolution, you can only view the external display (internal display will "white out"). |
| <b>Test Set IO</b>          |                                                                                                                                                                                                                    |
|                             | 25-pin D-Sub connector, female, available for external test set control                                                                                                                                            |
| <b>Aux IO</b>               |                                                                                                                                                                                                                    |

|                                                      |                                                                                                                                                      |
|------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                                      | 25-pin D-Sub connector, male, analog and digital IO                                                                                                  |
| <b>Handler IO</b>                                    |                                                                                                                                                      |
|                                                      | 36-pin parallel I/O port; all input/output signals are default set to negative logic; can be reset to positive logic via GPIB command female.        |
| <b>GPIB</b>                                          |                                                                                                                                                      |
|                                                      | 24-pin D-sub (Type D-24), female; compatible with IEEE-488.                                                                                          |
| <b>Parallel Port (LPT1)</b>                          |                                                                                                                                                      |
|                                                      | 25-pin D-Sub miniature connector, female; provides connection to printers or any other parallel port peripherals                                     |
| <b>Serial Port (COM 1)</b>                           |                                                                                                                                                      |
|                                                      | 9-pin D-Sub, male; compatible with RS-232                                                                                                            |
| <b>USB Port</b>                                      |                                                                                                                                                      |
|                                                      | One port on front panel and five ports on rear panel. Universal Serial Bus jack, Type A configuration (4 contacts inline, contact 1 on left); female |
| Contact 1                                            | Vcc: 4.75 to 5.25 VDC, 500 mA, maximum                                                                                                               |
| Contact 2                                            | -Data                                                                                                                                                |
| Contact 3                                            | +Data                                                                                                                                                |
| Contact 4                                            | Ground                                                                                                                                               |
| <b>LAN</b>                                           |                                                                                                                                                      |
|                                                      | 10/100BaseT Ethernet, 8-pin configuration; auto selects between the two data rates                                                                   |
| <b>Line Power</b> (A third-wire ground is required.) |                                                                                                                                                      |
| Frequency                                            | 48 Hz to 66 Hz                                                                                                                                       |
| Voltage at 115 V Setting                             | 90 to 132 VAC; 120 VAC, nominal                                                                                                                      |
| Voltage at 220 V Setting                             | 198 to 264 VAC; 240 VAC, nominal                                                                                                                     |
| VA Max                                               | 600 VA maximum                                                                                                                                       |

**Note:** Option H08 and Option H11 are not available with the N5230A network analyzer.

**Table 15.** Analyzer Environment and Dimensions

| Description                              | Supplemental Information                                                                                                                                                                                                                             |
|------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>General Environmental</b>             |                                                                                                                                                                                                                                                      |
| RFI/EMI Susceptibility                   | Defined by CISPR Pub. 11, Group 1, Class A, and IEC 50082-1                                                                                                                                                                                          |
| ESD                                      | Minimize using static-safe work procedures and an antistatic bench mat                                                                                                                                                                               |
| Dust                                     | Minimize for optimum reliability                                                                                                                                                                                                                     |
| <b>Operating Environment</b>             |                                                                                                                                                                                                                                                      |
| Temperature                              | 0 °C to +40 °C<br>Instrument powers up and displays no error messages within this temperature range (except for "source unlevelled" error message that may occur at temperatures outside the specified performance temperature range of 25 +/- 5°C). |
| Error-Corrected Temperature Range        | 23°C ± 3°C<br>with less than 1°C deviation from calibration temp.                                                                                                                                                                                    |
| Humidity                                 | 5% to 95% at +40 °C                                                                                                                                                                                                                                  |
| Altitude                                 | 0 to 4500 m (14,760 ft.)                                                                                                                                                                                                                             |
| <b>Non-Operating Storage Environment</b> |                                                                                                                                                                                                                                                      |
| Temperature                              | -40 °C to +70 °C                                                                                                                                                                                                                                     |
| Humidity                                 | 0% to 90% at +65 °C (non-condensing)                                                                                                                                                                                                                 |
| Altitude                                 | 0 to 4500 m (14,760 ft.)                                                                                                                                                                                                                             |

| <b>Cabinet Dimensions</b>                                                   |                          |                    |                    |
|-----------------------------------------------------------------------------|--------------------------|--------------------|--------------------|
|                                                                             | Height                   | Width              | Depth              |
| Excluding front and rear panel hardware and feet                            | 267 mm<br>10.5 in        | 426 mm<br>16.75 in | 427 mm<br>16.8 in  |
| As shipped - includes front panel connectors, rear panel bumpers, and feet. | 280 mm<br>11.0 in        | 435 mm<br>17.1 in  | 470 mm<br>18.5 in  |
| As shipped plus handles                                                     | 280 mm<br>11.0 in        | 458 mm<br>18 in    | 501 mm<br>19.7 in  |
| As shipped plus rack-mount flanges                                          | 280 mm<br>11.0 in        | 483 mm<br>19 in    | 470 mm<br>18.5 in  |
| As shipped plus handles and rack-mount flanges                              | 280 mm<br>11.0 in        | 483 mm<br>19 in    | 501 mm<br>19.70 in |
| <b>Weight</b>                                                               |                          |                    |                    |
| <b>Net</b>                                                                  | 24.9 kg (55 lb), nominal |                    |                    |
| <b>Shipping</b>                                                             | 36.3 kg (80 lb), nominal |                    |                    |

## Measurement Throughput Summary

### Typical Cycle Time for Measurement Completion

#### Cycle Time vs IF Bandwidth

#### Cycle Time vs Number of Points

#### Data Transfer Time

**Table 16** Typical Cycle Time<sup>a</sup> (ms) for Measurement Completion

| Description                                             | Typical Performance |       |       |       |        |
|---------------------------------------------------------|---------------------|-------|-------|-------|--------|
|                                                         | Number of Points    |       |       |       |        |
|                                                         | 201                 | 401   | 801   | 1601  | 16,001 |
| <b>Start 8 GHz, Stop 18 GHz, 600 kHz IF bandwidth</b>   |                     |       |       |       |        |
| Uncorrected                                             | 26.2                | 26.7  | 27.6  | 29.2  | 76.5   |
| 4-Port cal                                              | 93.0                | 104.1 | 125.2 | 164.0 | 939.6  |
| <b>Start 300 kHz, Stop 10 GHz, 600 kHz IF bandwidth</b> |                     |       |       |       |        |
| Uncorrected                                             | 24.8                | 28.0  | 30.4  | 35.0  | 91.8   |
| 4-Port cal                                              | 87.5                | 109.0 | 134.6 | 180.5 | 990.8  |
| <b>Start 300 kHz, Stop 20 GHz, 600 kHz IF bandwidth</b> |                     |       |       |       |        |
| Uncorrected                                             | 38.3                | 40.2  | 43.6  | 46.6  | 93.8   |
| 4-Port cal                                              | 140.2               | 158.3 | 190.0 | 224.2 | 1012.3 |
| <b>Start 8 GHz, Stop 18 GHz, 100 kHz IF bandwidth</b>   |                     |       |       |       |        |
| Uncorrected                                             | 43.1                | 56.9  | 60.9  | 62.1  | 193.4  |
| 4-Port cal                                              | 160.4               | 222.2 | 248.8 | 274.5 | 1291.1 |
| <b>Start 300 kHz, Stop 10 GHz, 100 kHz IF bandwidth</b> |                     |       |       |       |        |
| Uncorrected                                             | 41.8                | 48.3  | 51.1  | 53.7  | 209.9  |
| 4-Port cal                                              | 155.1               | 180.0 | 214.2 | 260.5 | 1362.7 |
| <b>Start 300 kHz, Stop 20 GHz, 100 kHz IF bandwidth</b> |                     |       |       |       |        |
| Uncorrected                                             | 51.4                | 76.4  | 94.0  | 99.8  | 211.4  |
| 4-Port cal                                              | 190.3               | 292.4 | 379.8 | 419.8 | 1378.7 |

| Start 8 GHz, Stop 18 GHz, 50 kHz IF bandwidth   |       |       |       |       |        |
|-------------------------------------------------|-------|-------|-------|-------|--------|
| Uncorrected                                     | 47.1  | 75.1  | 94.6  | 97.3  | 380.9  |
| 4-Port cal                                      | 171.6 | 290.1 | 381.0 | 410.0 | 1894.4 |
| Start 300 kHz, Stop 10 GHz, 50 kHz IF bandwidth |       |       |       |       |        |
| Uncorrected                                     | 49.1  | 67.2  | 72.7  | 75.9  | 395.1  |
| 4-Port cal                                      | 180.0 | 261.4 | 293.1 | 330.6 | 1941.2 |
| Start 300 kHz, Stop 20 GHz, 50 kHz IF bandwidth |       |       |       |       |        |
| Uncorrected                                     | 54.9  | 87.1  | 131.2 | 154.4 | 396.3  |
| 4-Port cal                                      | 207.0 | 337.7 | 523.9 | 633.6 | 1948.2 |

<sup>a</sup> Includes sweep time, retrace time and band-crossing time. Analyzer display turned off with DISPLAY:ENABLE OFF. Add 21 ms for display on. Data for one trace (S<sub>11</sub>) measurement.

**Table 17. Cycle Time vs IF Bandwidth**

Applies to the Preset condition (201 points, correction off) except for the following changes:

- CF = 10 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Description       | Typical Performance          |             |
|-------------------|------------------------------|-------------|
|                   | Cycle Time (ms) <sup>a</sup> | Trace Noise |
| IF Bandwidth (Hz) |                              |             |
| 600,000           | 7.523394495                  | 0.003533948 |
| 360,000           | 7.54179941                   | 0.002688865 |
| 280,000           | 7.5703125                    | 0.002287365 |
| 200,000           | 7.71344                      | 0.002102872 |
| 150,000           | 7.762206897                  | 0.001696417 |
| 100,000           | 7.806733333                  | 0.001284263 |
| 70,000            | 7.874966555                  | 0.001170092 |
| 50,000            | 9.076777778                  | 0.000987238 |
| 30,000            | 11.46182377                  | 0.0008445   |
| 20,000            | 14.72636574                  | 0.000647383 |



|        |             |             |
|--------|-------------|-------------|
| 15,000 | 17.5863125  | 0.000534657 |
| 10,000 | 28.64310448 | 0.000477914 |
| 7000   | 37.16706481 | 0.000439644 |
| 5000   | 48.58746512 | 0.000350175 |
| 3000   | 72.52639344 | 0.00030881  |
| 2000   | 102.2277778 | 0.000279538 |
| 1500   | 130.7245    | 0.00015128  |
| 1000   | 218.5535    | 0.000154337 |
| 700    | 294.1385333 | 0.000135211 |
| 500    | 399.9245455 | 0.000125675 |
| 300    | 636.411     | 0.000103409 |
| 200    | 932.7632    | 0           |
| 100    | 1826.966667 | 0           |
| 30     | 6004.446    | 0           |
| 10     | 17903.564   | 0           |
| 1      | 178398.611  | 0           |

a Cycle time includes sweep and retrace time.

**Table 18. Cycle Time vs Number of Points**

Applies to the Preset condition (correction off) except for the following changes:

- CF = 10 GHz
- Span = 100 MHz
- Display off (add 21 ms for display on)

| Description       | Typical Performance |                              |
|-------------------|---------------------|------------------------------|
|                   | Number of Points    | Cycle Time (ms) <sup>a</sup> |
| IF Bandwidth (Hz) |                     |                              |

|         |        |       |
|---------|--------|-------|
| 30,000  | 3      | 6.7   |
|         | 11     | 7.4   |
|         | 51     | 6.9   |
|         | 101    | 7.8   |
|         | 201    | 11.2  |
|         | 401    | 18.3  |
|         | 801    | 32.4  |
|         | 1,601  | 59.4  |
|         | 6,401  | 224.7 |
|         | 16,001 | 556.9 |
| 100,000 | 3      | 6.7   |
|         | 11     | 6.6   |
|         | 51     | 6.8   |
|         | 101    | 7     |
|         | 201    | 7.5   |
|         | 401    | 9     |
|         | 801    | 13.5  |
|         | 1,601  | 22.9  |
|         | 6,401  | 75.3  |
|         | 16,001 | 180.3 |
| 600,000 | 3      | 6.5   |
|         | 11     | 6.6   |
|         | 51     | 6.8   |
|         | 101    | 6.9   |
|         | 201    | 7.3   |
|         | 401    | 8.1   |
|         | 801    | 9.4   |
|         | 1,601  | 12    |
|         | 6,401  | 27.7  |
|         | 16,001 | 59.3  |

a Cycle time includes sweep and retrace time.

**Table 19. Data Transfer Time (ms)**

| Description                                                 | Typical Performance |     |      |        |
|-------------------------------------------------------------|---------------------|-----|------|--------|
|                                                             | Number of Points    |     |      |        |
|                                                             | 201                 | 401 | 1601 | 16,001 |
| <b>SCPI over GPIB<br/>(program executed on external PC)</b> |                     |     |      |        |
| 32-bit floating point                                       | 7                   | 12  | 43   | 435    |
| 64-bit floating point                                       | 12                  | 22  | 84   | 856    |
| ASCII                                                       | 64                  | 124 | 489  | 5054   |
| <b>SCPI<br/>(program executed in the analyzer)</b>          |                     |     |      |        |
| 32-bit floating point                                       | 1                   | 2   | 3    | 30     |
| 64-bit floating point                                       | 2                   | 2   | 4    | 40     |
| ASCII                                                       | 29                  | 56  | 222  | 2220   |
| <b>COM (program executed in the analyzer)</b>               |                     |     |      |        |
| 32-bit floating point                                       | <0.4                | 0.4 | 0.5  | 1.9    |
| Variant type                                                | 0.7                 | 1   | 3    | 32     |
| <b>DCOM over LAN<br/>(program executed on external PC)</b>  |                     |     |      |        |
| 32-bit floating point                                       | <0.8                | 1   | 1.5  | 7.1    |
| Variant type                                                | 1.8                 | 2.7 | 8.5  | 80     |

---


**Note:** Specifications for Recall & Sweep Speed are not provided for the N5230A analyzers.

---


## **Tables 20 - 25 Front-panel Jumper Specs (Option 245 only)**

### **Test Set Block Diagrams**

#### **N5230A Option 240 (Standard Test Set and Standard Power Range)**

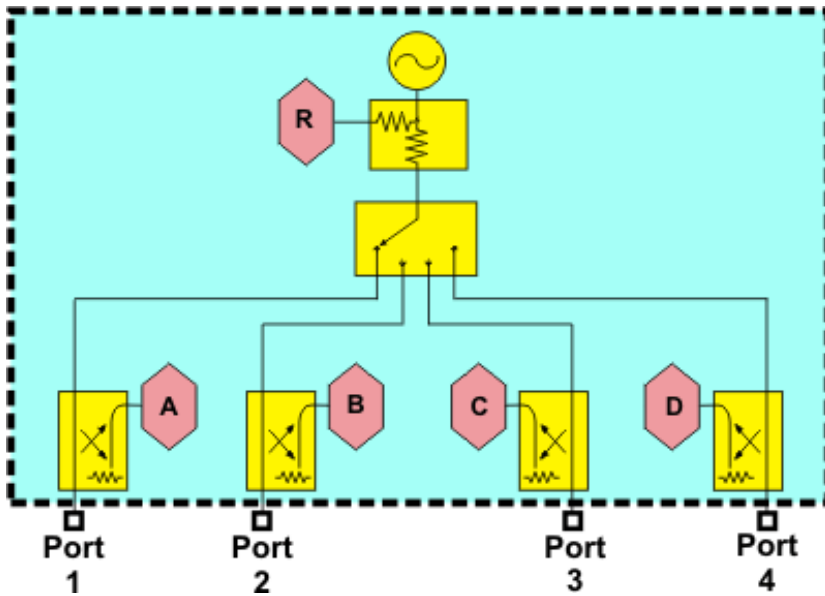

N5230A Option 245 (Configurable Test Set and Extended Power Range)

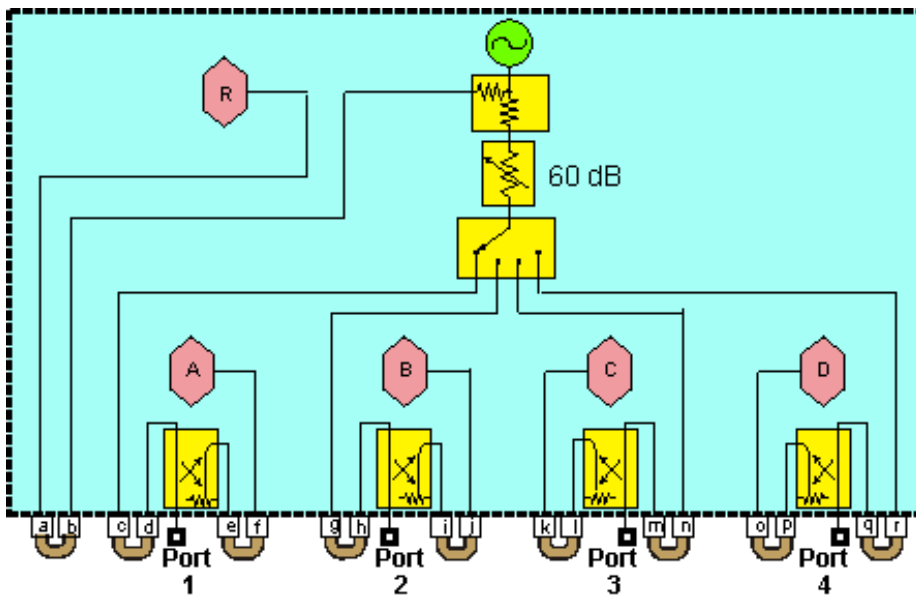

| Item | Description | Item | Description | Item | Description |
|------|-------------|------|-------------|------|-------------|
| a    | RCVR R IN   | h    | CPLR THRU   | o    | RCVR D IN   |
| b    | SOURCE OUT  | i    | CPLR ARM    | p    | CPLR ARM    |
| c    | SOURCE OUT  | j    | RCVR B IN   | q    | CPLR THRU   |
| d    | CPLR THRU   | k    | RCVR C IN   | r    | SOURCE OUT  |
| e    | CPLR ARM    | l    | CPLR ARM    |      |             |
| f    | RCVR A IN   | m    | CPLR THRU   |      |             |
| g    | SOURCE OUT  | n    | SOURCE OUT  |      |             |

## Typical System Performance for the N5250A

(Rev. 2004-08-02)

- This is a complete list of the N5250A network analyzer typical system performance.
- To view or print the .pdf version of this document, visit our web site at <http://www.agilent.com>, type 5988-9620EN in the Quick Search box, then click GO.

**See Specs for other PNA models**

### Definitions

**Typical** : Expected performance of an average unit which does not include guardbands. It is not covered by the product warranty.

**Standard**: When referring to the analyzer, this includes no options unless noted otherwise.

Unlike the lengthy specifications documents for other PNA models, this document presents typical system performance for the following categories only:

- System Dynamic Range
- Test Port Power
- Noise Floor
- Test Port Damage Level
- Option H11 Rear Panel Connectors

### Typical System Performance

Table 1. System Dynamic Range

| Frequency         | 1.0 mm Test Port | 1.85 mm PNA Test Port | Waveguide Port |
|-------------------|------------------|-----------------------|----------------|
| 10 MHz to 45 MHz  | 63 dB            | 65 dB                 |                |
| 45 MHz to 500 MHz | 94 dB            | 97 dB                 |                |
| 500 MHz to 2 GHz  | 120 dB           | 123 dB                |                |
| 2 GHz to 10 GHz   | 116 dB           | 123 dB                |                |
| 10 GHz to 24 GHz  | 111 dB           | 121 dB                |                |
| 24 GHz to 30 GHz  | 100 dB           | 112 dB                |                |
| 30 GHz to 40 GHz  | 92 dB            | 107 dB                |                |
| 40 GHz to 45 GHz  | 84 dB            | 101 dB                |                |

|                    |       |        |        |
|--------------------|-------|--------|--------|
| 45 GHz to 50 GHz   | 85 dB | 103 dB |        |
| 50 GHz to 60 GHz   | 80 dB | 100 dB |        |
| 60 GHz to 67 GHz   | 75 dB | 95 dB  |        |
| 67 GHz to 70 GHz   | 68 dB |        | 82 dB  |
| 70 GHz to 75 GHz   | 74 dB |        | 87 dB  |
| 75 GHz to 80 GHz   | 85 dB |        | 98 dB  |
| 80 GHz to 100 GHz  | 89 dB |        | 101 dB |
| 100 GHz to 110 GHz | 87 dB |        | 98 dB  |

**Table 2.** Test Port Power

| <b>Frequency</b>   | <b>1.0 mm Test Port<br/>(Std Configuration<sup>a</sup> or<br/>Opt 017<sup>b</sup>)</b> | <b>1.85 mm PNA Port</b> | <b>Waveguide<br/>Port</b> |
|--------------------|----------------------------------------------------------------------------------------|-------------------------|---------------------------|
| 10 MHz to 45 MHz   | -8 dBm                                                                                 | -7 dBm                  |                           |
| 45 MHz to 500 MHz  | -3 dBm                                                                                 | -1 dBm                  |                           |
| 500 MHz to 2 GHz   | 0 dBm                                                                                  | 2 dBm                   |                           |
| 2 GHz to 10 GHz    | -2 dBm                                                                                 | 2 dBm                   |                           |
| 10 GHz to 24 GHz   | -5 dBm                                                                                 | 0 dBm                   |                           |
| 24 GHz to 30 GHz   | -7 dBm                                                                                 | 0 dBm                   |                           |
| 30 GHz to 40 GHz   | -10 dBm                                                                                | -1 dBm                  |                           |
| 40 GHz to 45 GHz   | -15 dBm                                                                                | -5 dBm                  |                           |
| 45 GHz to 50 GHz   | -12 dBm                                                                                | -1 dBm                  |                           |
| 50 GHz to 60 GHz   | -17 dBm                                                                                | -4 dBm                  |                           |
| 60 GHz to 67 GHz   | -22 dBm                                                                                | -8 dBm                  |                           |
| 67 GHz to 70 GHz   | -9 dBm                                                                                 |                         | -2 dBm                    |
| 70 GHz to 75 GHz   | -7 dBm                                                                                 |                         | 0 dBm                     |
| 75 GHz to 80 GHz   | -6 dBm                                                                                 |                         | +1 dBm                    |
| 80 GHz to 100 GHz  | -5 dBm                                                                                 |                         | +1 dBm                    |
| 100 GHz to 110 GHz | -8 dBm                                                                                 |                         | -2 dBm                    |

a Assumes a 30" cable from the PNA 1.85mm Test Port Out is used to provide the 10 MHz to 67 GHz source signal. The Standard configuration does not have a bias tee in the 1.0mm head.

b Assumes a 30" cable from the PNA Source Out bulkhead connector is used to provide the 10 MHz to 67 GHz source signal. Option 017 includes a bias tee in the 1.0mm head.

**Table 3:** Noise Floor

| Frequency          | 1.0mm Test Port | 1.85mm Test Port | Waveguide Port |
|--------------------|-----------------|------------------|----------------|
| 10 MHz to 45 MHz   | -71 dBm         | -72 dBm          |                |
| 45 MHz to 500 MHz  | -97 dBm         | -98 dBm          |                |
| 500 MHz to 2 GHz   | -120 dBm        | -121 dBm         |                |
| 2 GHz to 10 GHz    | -118 dBm        | -121 dBm         |                |
| 10 GHz to 24 GHz   | -116 dBm        | -121 dBm         |                |
| 24 GHz to 30 GHz   | -107 dBm        | -112 dBm         |                |
| 30 GHz to 40 GHz   | -102 dBm        | -108 dBm         |                |
| 40 GHz to 45 GHz   | -99 dBm         | -106 dBm         |                |
| 45 GHz to 50 GHz   | -97 dBm         | -104 dBm         |                |
| 50 GHz to 60 GHz   | -97 dBm         | -104 dBm         |                |
| 60 GHz to 67 GHz   | -92 dBm         | -103 dBm         |                |
| 67 GHz to 70 GHz   | -77 dBm         |                  | -84 dBm        |
| 70 GHz to 75 GHz   | -81 dBm         |                  | -87 dBm        |
| 75 GHz to 80 GHz   | -91 dBm         |                  | -97 dBm        |
| 80 GHz to 100 GHz  | -94 dBm         |                  | -100 dBm       |
| 100 GHz to 110 GHz | -95 dBm         |                  | -100 dBm       |

**Table 4.** Test Port Damage Level

| Frequency         | 1.0mm Test Port | 1.85mm Test Port | Waveguide Port |
|-------------------|-----------------|------------------|----------------|
| 10 MHz to 110 GHz | 27 dBm          | 27 dBm           | 27 dBm         |

**Table 5** Option H08 & H11 Rear Panel Connectors (typical)

|                                                                                                            |                                                                                |
|------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------|
| IF Connectors                                                                                              | A, R1, R2, B (BNC Connectors)                                                  |
| IF Connector Input Frequency                                                                               | 8 1/3 MHz                                                                      |
| Nominal Input Impedance at IF Inputs                                                                       | 50 $\Omega$                                                                    |
| RF Damage Level to IF Connector Inputs                                                                     | -20.0 dBm                                                                      |
| DC Damage Level to IF Connector Inputs                                                                     | 25 volts                                                                       |
| 0.1 dB Compression Point at IF Inputs                                                                      | -27.0 dBm                                                                      |
| Pulse Input Connectors <sup>1</sup>                                                                        | A, R1, R2, B (BNC Connectors)                                                  |
| Nominal Input Impedance at Pulse Inputs                                                                    | 1 Kohm                                                                         |
| Minimum IF Gate Width                                                                                      | 20 ns for less than 1 dB deviation from theoretical performance <sup>2</sup> . |
| DC Damage Level to Pulse Connector Inputs                                                                  | 5.5 volts                                                                      |
| Drive Voltage                                                                                              | TTL (0, +5.0) Volts                                                            |
| Rear Panel LO Power – Test Port Frequency<br>(see 836x H11 Specs for Test Port Frequencies up to 67 GHz)   |                                                                                |
| 67 GHz to 110 GHz <sup>3</sup>                                                                             | -7 to -13 dBm                                                                  |
| Rear Panel RF Power - Test Port Frequencies<br>(see 836x H11 Specs for Test Port Frequencies up to 67 GHz) |                                                                                |
| 67 GHz to 76 GHz <sup>4</sup>                                                                              | -4 to -10 dBm                                                                  |
| 76 GHz to 96 GHz <sup>4</sup>                                                                              | +1 to -5 dBm                                                                   |
| 96 GHz to 110 GHz <sup>4</sup>                                                                             | +5 to -1 dBm                                                                   |

1 Pulse input connectors are operational only with Option H08 (Pulse Measurement Capability) enabled.

2 Based on deviation from signal reduction equation: Signal Reduction (dB) =  $20\log_{10}(\text{Duty\_cycle}) = 20\log_{10}(\text{pulse\_width/period})$ . Measured at Pulse Repetition Frequency (PFR) of 1 MHz.

3 For rear panel LO port frequency, divide by 8

4 For rear panel RF port frequency, divide by 6


---

Note: Typical system performance for front panel jumpers is not provided for the N5250A.



## Test Set Block Diagram


N5250A - Standard Network Analyzer

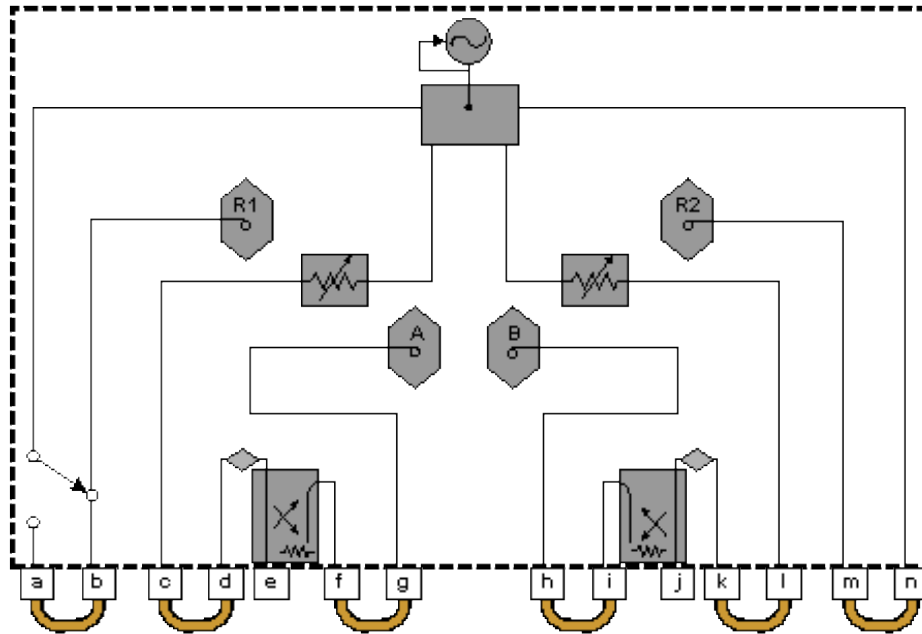

| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

## Test Set with Option 016 Block Diagram

N5250A - Option 016 Receiver Attenuators Network Analyzer

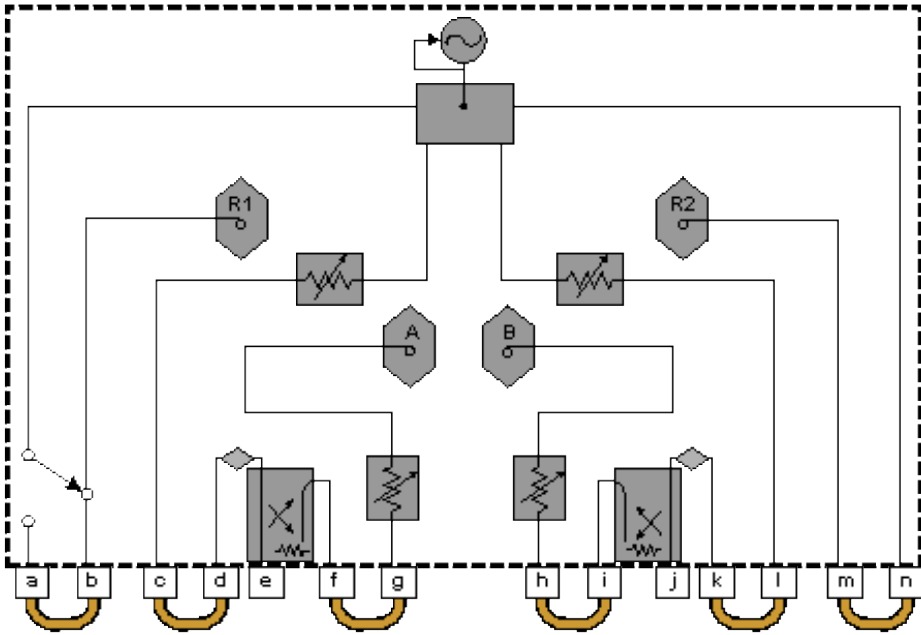

| Item | Description | Item | Description |
|------|-------------|------|-------------|
| a    | SOURCE OUT  | h    | RCVR B IN   |
| b    | RCVR R1 IN  | i    | CPLR ARM    |
| c    | SOURCE OUT  | j    | PORT 2      |
| d    | CPLR THRU   | k    | CPLR THRU   |
| e    | PORT 1      | l    | SOURCE OUT  |
| f    | CPLR ARM    | m    | RCVR R2 IN  |
| g    | RCVR A IN   | n    | SOURCE OUT  |

## Glossary

[A](#)   [B](#)   [C](#)   [D](#)   [E](#)   [F](#)   [G](#)   [H](#)   [I](#)   [J](#)   [K](#)   [L](#)   [M](#)  
[N](#)   [O](#)   [P](#)   [Q](#)   [R](#)   [S](#)   [T](#)   [U](#)   [V](#)   [W](#)   [X](#)   [Y](#)   [Z](#)

---

**12-Term Error Correction** See [Error Correction, 12-Term](#).

**1-Port Device** A device with a single connector or path to the device's circuitry. Examples include an oscillator and a load.

**2-Port Calibration, Full** See [Error Correction, 12-Term](#).

**2-Port Device** A device with two connectors or other paths to the device's circuitry. Examples include filters, SAW devices, attenuators, matching pads, and amplifiers.

**3-Term Error Correction** See [Error Correction, 3-Term](#).

---

## A

**Active Channel** The highlighted channel affected by front panel functions.

**Active Function Readout** The area of a display screen where the active function and its state are displayed. The active function is the one that was completed by the last key selection or remote programming command.

**Active Marker** The marker on a trace that can be repositioned either by front panel controls or by programming commands.

**Active Trace** A trace that is being swept (updated) with incoming signal information.

**ADC** Analog to Digital Converter

**Address** The identification (represented by a name, label, or number) for a register, location in storage, or any other data source or destination. Examples are the location of a station in a communications network, or a device on the GP-IB.

**ADM** Add-Drop Multiplexer

**Admittance (Y)** The inverse of an impedance (i.e. the ratio of current to voltage). Complex admittances take the form  $Y = G + jB(t)$ .

**ALC** Automatic Level Control. See [Automatic Gain Control](#).

 **AM** Amplitude Modulation

**AM Group Delay** A technique for the measurement of group delay through a device which utilizes an amplitude modulated (AM) source. Note: The actual delay of the modulation envelope is measured directly with an external scalar detector. Devices that distort the amplitude of a signal cannot be measured. These include amplifiers with automatic gain control (AGC) and devices subject to saturation or power limiting.

**Amplitude Modulation** The process, or result of the process, of varying the amplitude of a carrier signal. The resulting modulated carrier contains information that can be recovered by demodulation. See also [Modulation](#).

**Analog** The general class of devices or circuits in which the output varies as a continuous function of the input.

**Annotation** The labeling of specific information on the display (such as frequency or power).

**ANSI** American National Standards Institute: A national membership organization (open to manufacturers, organizations, users, and communications carriers) that approves standards, accredits standards development groups and certificate programs, and represents and coordinates US interests in non-treaty and non-government standards bodies.

**Aperture** The frequency span of the network analyzer used for calculating group delay. The narrower the aperture, the finer the resolution of the group delay variations, but noise is reduced by increasing the aperture.

**Array** A set of numbers or characters that represents any given function.

**ASCII** American Standard Code for Information Interchange

**Attenuation** Denotes a reduction in signal amplitude. The difference between transmitted and received power due to loss through equipment, lines, or other transmission devices; usually expressed in decibels.

**Attenuator** An RF or microwave device used to reduce the power level of a signal by precise, incremental amounts over its entire frequency range.

**Automatic Calibration System** AutoCal: Feature offered on Rohde&Schwarz network analyzers.

**Automatic Gain Control (AGC)** A circuit used in amplifiers and other active devices to keep its RF power level constant as other parameters change, such as frequency. Synonym: Automatic Leveling Control (ALC)

**Autoscale** An analyzer feature that evaluates waveforms and adjusts controls to stable and enhance the display.

**AUX** Auxiliary; refers to rear-panel input connector.

**Averaging** A noise reduction technique that computes each data point based on consecutive sweeps and weighted by a user-specified averaging factor. Each new sweep is averaged into the trace until the total number of sweeps is equal to the averaging factor.

---

## B

**B/R** The ratio of data sampled at B to the data sampled at R.

**Band Pass** A range of frequencies that are passed through a device, such as a filter. Frequencies not within the band pass are limited or attenuated. See also [Cutoff Frequency](#).

**Bandwidth (BW)** The difference between the frequencies of a continuous frequency band within which performance of a device falls within specifications.

**Bandwidth Limit** The condition prevailing when the system bandwidth is exceeded and signal distortion occurs beyond specifications.

**Bandwidth Selectivity** A measure of a filter's ability to resolve signals unequal in amplitude. It is the ratio of the 60 dB bandwidth to the 3 dB bandwidth for a given resolution filter (IF). Bandwidth selectivity tells us how steep the filter skirts are. Bandwidth selectivity is sometimes called shape factor.

**Binary** A method of representing numbers in a scale of two (on or off, high-level or low-level, one or zero). A compact, fast format used to transfer information to and from the analyzer.

**BMP** Bit-Mapped

**Brightness** See [Color Brightness](#).

**Broadband Device** A device that operates over a very wide frequency range and exhibits only small variations in response over that range.

**Buffer** A storage device used when transmitting information to compensate for a difference in the rate of flow of information between two devices.

**Burst Carrier** A carrier that is periodically turned off and on. A burst carrier may or may not be modulated.

**BUS** Basic Utility System

**Bus** One or more conductors used as a path to deliver transmitted information from any of several sources to any of several destinations.

**BW** Bandwidth

**Byte** Eight bits of data representing one character processed as a unit.

---

## C

**CAD** Computer Aided Design

**CAE** Computer Aided Engineering

**Calibration** In HP instrumentation, the process of periodically (usually annually) verifying an instrument is performing to specifications. A calibration certificate is awarded after verification.

In network analyzers, the process of removing systematic errors from measurements. See [Error Correction](#).

**Calibration Kit** Hardware and software required to perform error correction on a network analyzer for a specific measurement and/or test set.

**Calibration, 2-Port** See [Error Correction, 12-Term](#).

**Calibration, Blackburn** Calibrations of transmission path with corrected source match involving 15 calibration terms. Synonym: 15-term error correction

**Calibration, Frequency Response** The simplest error correction procedure to perform, but only corrects for a few of the twelve possible systematic error terms. Frequency response corrections can be made for reflection measurements, transmission measurements, and isolation measurements.

**Calibration, Interpolation** A user selectable network analyzer feature that calculates (interpolates) new error correction terms from existing terms when there is a change in network analyzer parameters, such as IF bandwidth, power, or sweep time. The resulting error correction is not as accurate as completing a full 2-port calibration.

**Calibration, Port Extension** See [Port Extension](#).

**Calibration, Reference Plane** See [Reference Plane](#).

**Calibration, Set Z** Sets the system impedance, usually 50 or 75 ohms.

**Calibration, SOLT** A calibration using four known standards: Short-Open-Load-Through. Also known as a full two-port calibration and 12-term error correction. See also [Error Correction](#).

**Calibration, TRL and LRM** A calibration used in environments where the DUT cannot be connected directly to the network analyzer ports, (MMIC, microstrip, beam-lead diodes etc.). Thru-Reflect-Line (TRL) and M (Match) standards are fabricated and used because known high-quality standards are not readily available. The requirements for characterizing these standards are less stringent, but the calibration is not as accurate as the traditional full two-port calibration using S-O-L-T standards. The terms are used interchangeably (TRL, LRL, LRM etc.) but they all refer to the same basic calibration method.

**Characteristic Impedance** The impedance looking into the end of an infinitely long lossless transmission line.

**Color Brightness** A measure of the intensity (brightness) of a color.

**Command** A set of instructions that are translated into instrument actions. The actions are usually made up of individual steps that together can execute an operation.

**Continuous Sweep Mode** The analyzer condition where traces are automatically updated each time trigger conditions are met.

**Controller** A device capable of specifying the talker and listeners for an information transfer. An external computer connected to an instrument to control its operation.

**Corrected** Measurements made after performing error correction.

**Coupler** See [Directional Coupler](#).

**CPU** Central Processing Unit

**Crosstalk** The occurrence of a signal at one port of a device being affected by a signal in any other path. Isolation is the measurement of crosstalk.

**Cursor** An electronically generated pointer that moves across the display to manipulate controls.

**Cutoff Frequency** In filters, the frequency at which attenuation is 3dB below the band pass signal level, known as the 3dB points.

**CW** Continuous wave: A single frequency (rather than a swept frequency).

---

## D

## **DAC** Digital to Analog Converter

**dB** Decibel: a relative unit of measure. The ratio in dB is given by:  $10 \log_{10} (P_1/P_2)$  where  $P_1$  and  $P_2$  are the measured powers. The dB is preferred instead of arithmetic ratios or percentages because when components are connected in series, their effect on power, expressed in dB, may be arithmetically added and subtracted. For example, if a 3dB attenuator is connected to a 10dB amplifier, the net gain of the two components is (-3dB + 10dB = +7dB).

**dBm** Absolute unit of measure in decibels: 0dBm = 1 mW. The conventions of the dB (adding and subtracting) continue to apply.

## **DBMS** Database Management System

## **DC** Direct Current

**Default** A known set of conditions used in the absence of user-defined conditions.

**Delay** See [Group Delay](#).

**Demodulation** The process of recovering from a modulated carrier, information in the form of a signal having essentially the same characteristics as the original modulating signal. Recovery of the modulating signal accomplished by signal detection.

**Detection** The process of demodulating signal carriers. There are two basic ways of providing signal detection in network analyzers: Diode detectors (used in broadband applications) and heterodyning, (used in narrowband applications).

**Detector, Diode** A device used to convert a RF signal to a proportional DC level. If the signal is amplitude modulated, the diode strips the RF carrier signal from the modulation. Many sources used with scalar analyzers are amplitude modulated with a 27.778 kHz signal and then detected in the network analyzer. Phase information on the signal carrier is lost in diode detection.

**Deviation from Linear Phase** Linear phase refers to the nature of the phase shift of a signal through a device. The phase is linear if a plot of phase shift versus frequency is a straight line using linear scales. Deviation from linear phase causes signal distortion.

**Digital** Pertaining to the class of devices or circuits in which the output varies in discrete steps.

**Digital Demodulation** Describes a technique of extracting the information used to modulate a signal. Digital signal processing algorithms are used on the signal after it has been converted from an analog to a digital form (digitized).

**Dimension** To specify the size of an array. The number of array rows or columns.

**Directivity** In a 3-port directional coupler, the ratio of the power present at the auxiliary port when the signal is traveling in the forward direction to the power present at the auxiliary port when the same signal is traveling in the reverse direction.

**Directional Coupler** A 3-port device typically used for separately sampling the backward (reflected) wave in a transmission line.

**Disk** A circular, magnetic storage medium.

**Display** Noun: See [Screen](#).

Verb: To show annotation and measurement data on the display.

**Display Detector Mode** The manner in which analog, video information is processed prior to being digitized and stored in memory.

**Display Dynamic Accuracy** The amplitude uncertainty, usually in dB, over the display dynamic range.

**Display Dynamic Range** The amplitude range, in dB, over which the display dynamic accuracy applies.

**Display Formats** Graphical formats for displaying measurement data. These include single channel, overlay (multiple traces on one graticule), split (each trace on separate graticules).

**Display Modes** The ways in which measurement data can be presented graphically. On a network analyzer, the choices are Cartesian/rectilinear (XY plot with log or linear magnitude, phase, group delay, SWR, real and imaginary, and dBV, dBmV and dBuV), polar (magnitude and angle), magnitude and phase, and Smith chart. Not

all display modes are available on all network analyzers. In addition, displays can present this information in various combinations of traces. Common modes are dual, (the ability to display more than one trace, usually over the same frequency range), and alternate, (the ability to display more than one trace, each with different frequency range and type).

**Display Phase Dynamic Accuracy** The phase measurement uncertainty, usually in degrees, for measurements whose units are in degrees.

**Display Points** The total number of measurement points made in a single measurement. The points can be in units of frequency, power, or time. The number of points often dictates measurement speed, resolution, and aperture.

**Display Trace Noise, Magnitude** The amplitude uncertainty of the trace, in dB, due to random noise in the test system.

**Display Trace Noise, Phase** The phase uncertainty of the trace, in degrees, due to random noise in the test system.

**Display Type** The type of display screen built into the analyzer. Data can be displayed as a raster drawing (a computer-like dot map) or as a vector drawing (lines drawn on the display). Color and display standard can also be specified as monochrome (single color), or color (two or more colors). The format standard may also be specified, such as VGA or SVGA, for IBM-compatible personal computers.

**Distortion** Deterioration of a signal's quality due to the nonlinear characteristics of a device or system transfer function. Distortion is measured as a combination of the changes in amplitude, frequency and phase of signal at the output of a device or system as compared to the signal at the input.

**Drift** The slow change in signal frequency.

**DSP** Digital Signal Processing

**DUT** Device Under Test

**DVM** Digital Volt Meter

**Dynamic Range** In a receiver, the range of signal levels, from minimum to maximum, that can be reliably measured simultaneously. Dynamic range allows small signals to be measured in the presence of large signals. Source power and receiver compression usually limits the maximum boundary to dynamic range. Receiver residual responses and noise floor usually limit the minimum power boundary.

---

## E

**ECal** See [Electronic Calibration](#).

**Electrical Delay** A simulated variable length of lossless transmission line, added to or subtracted from a receiver input, to compensate for interconnecting cables. The firmware equivalent of mechanical or analog "line stretchers" in other network analyzers.

**Electronic Calibration (ECal)** A calibration system for electronic calibration of RF and microwave vector network analyzers. The electronic calibration system creates a twelve-term, two-port error model and then provides a confidence check of the calibration. The Ecal system consists of a repeatable, variable-impedance, solid-state calibration standard and a mainframe control unit which interfaces with the 8510, 8720 series, and the 8753 network analyzers or a USB module which interfaces with the PNA series network analyzers.

**EMC** Electro-Magnetic Compatibility

**EMI** Electro-Magnetic Interference: Unintentional interfering signals generated within or external to electronic equipment. Typical sources could be power-line transients, noise from switching-type power supplies and/or spurious radiation from oscillators. EMI is suppressed with power-line filtering, shielding, etc.

**Engage** To activate a function.

**Enter** The process of inputting information.

**EPROM** Electronically Programmable, Read-Only Memory

**Error Correction** In network analyzers, a process that removes or reduces systematic (repeatable) measurement

errors by measuring known standards from a calibration kit. Synonym: measurement calibration

**Error Correction, 3-Term** Used to remove systematic measurement errors on a device with one port, such as a load.

**Error Correction, 12-Term** Correction for a two port device using six parameters:

Directivity

Source match

Load match

Reflection frequency response

Transmission frequency response

Isolation

To completely characterize a two-port device, these six parameters must be characterized in the forward and reverse directions, making a total of 12 terms. The user usually has the option of omitting isolation from the correction process. Synonym: Full two-port error correction

**Error Correction, 1-Port** Corrects a test set for port 1 or port 2 directivity, frequency response, and source match errors. The process requires three known standard terminations, for example, open, short, and load.

**Error Message** A message on a display that indicates an error condition. Missing or failed hardware, improper user operation, or other conditions that require additional attention can cause an error condition. Generally, the requested action or operation cannot be completed until the condition is resolved.

**ESD** Electro Static Discharge

**Ethernet** A network that adheres to the IEEE 802.3 Local Area Network standard.

**Ethernet address** A hexadecimal number which is used to identify a machine on a network. Each analyzer is assigned a unique Ethernet address at the factory and it is stored in the analyzer's ROM.

**External trigger signal** A TTL signal that is input to an analyzer and initiates a measurement sweep or similar event, making the measurements synchronous with the external triggering source.

---

## F

**Filter** A passive device that allows some frequencies to pass and attenuates others, depending on the type and specifications. A high-pass filter passes frequencies above the cutoff frequency, a low-pass filter passes frequencies below the cutoff frequency, and a band-pass filter passes frequencies between two specific frequencies.

**Firmware** An assembly made up of hardware and instruction code. The hardware and instruction code is integrated and forms a functional set that cannot be altered during normal operation. The instruction code, permanently installed in the circuitry of the instrument, is classified as ROM (read only memory). The firmware determines the operating characteristics of the instrument or equipment.

**Flatness** The amplitude and phase response of a device under test (DUT), a signal source, a receiver, or a combination of these. See also [Frequency Response](#).

**FM** Frequency Modulation

**Frequency** The number of periodic oscillations, vibrations, or waves per unit of time, usually expressed in cycles per second, or Hertz (Hz).

**Frequency Accuracy** The uncertainty with which the frequency of a signal or spectral component is indicated, either in an absolute sense or relative to another signal or spectral component. Absolute and relative frequency accuracies are specified independently.

**Frequency Range** The range of frequencies over which a device or instrument performance is specified.

**Frequency Resolution** The ability of a network analyzer to measure device characteristics at closely spaced frequencies and display them separately. Resolution of equal amplitude responses is determined by IF bandwidth. Resolution of unequal amplitude responses is determined by IF bandwidth and bandwidth selectivity.

**Frequency Response** The peak-to-peak variation in the displayed amplitude response over a specified center frequency range. Frequency response is typically specified in terms of dB, relative to the value midway between the



extremes.

**Frequency Span** The magnitude of the displayed frequency component. Span is represented by the horizontal axis of the display. Generally, frequency span is given as the total span across the full display. Some analyzers represent frequency span (scan width) as a per-division value.

**Frequency Stability** The ability of a frequency component to remain unchanged in frequency or amplitude over short and long-term periods of time. Stability refers to an oscillator's ability to remain fixed at a particular frequency over time.

**Front Panel Key** Keys that are located on the front panel of an instrument. The key labels identify the function the key activities. Numeric keys and step keys are two examples of front panel keys.

**Full 2-Port Calibration** See [Error Correction, 12-Term](#).

**Function** The action or purpose that a specific item is intended to perform or serve. The network analyzer contains functions that can be executed via front panel key selections, or through programming commands. The characteristics of these functions are determined by the firmware in the instrument. In some cases, a DLP (downloadable program) execution of a function allows you to execute the function from front panel key selections.

**Fundamental Frequency** In any waveform, the lowest frequency component; all other components are harmonics. A pure sinusoid has only one component, the fundamental.

---

## G

**Gb** Gigabit

**GB** Gigabyte

**GHz** Gigahertz

**GIF** Graphics Interchange Format - Standard graphic format to store bitmapped graphics files.

**Giga** Prefix for one billion.

**GP I/O** General Purpose Input / Output; a connector usually on the back of an instrument that allows communication with other test equipment, external test sets, switches, and computers that enable the instrument to be triggered or to trigger external equipment. An example is a foot switch that continues or cycles a measurement, allowing the operator to use both hands on the test hardware.

**GPIB** General Purpose Interface Bus - IEEE 488 bus is interconnect bus and protocol, allows linking of instruments and computer.

**Graticule (or Grid)** Enclosed area where waveform is displayed on instrument. Tick marks, on frame or axis, are a scaling aid for making visual measurements.

**Group Delay** A measure of the transit time of a signal through a DUT versus frequency. Group delay can be calculated by differentiating the DUT's insertion-phase response with respect to frequency. See also [AM Group Delay](#) and [Deviation from Linear Phase](#).

**GUI** Graphical User Interface

---

## H

**Hardcopy** Paper copy of data.

**Hardkey** A front-panel key, which engages a single analyzer function or presents a single menu of softkeys.

**Horizontal Reference** See [Reference Level](#).

**Horizontal Resolution** The analyzer's ability to take closely spaced horizontal data points over the full sweep.

**Host Computer** A computer or device on a network that provides end users with services such as computation and database access and that usually performs network control functions.

**Host Name** A unique name that is used to identify each host machine on a network. The host name is directly linked to, and can usually be used in place of, the IP address. The user or the system administrator usually creates

the host name.

**HP** Hewlett-Packard Company

**HPGL** Hewlett-Packard Graphics Language

**HP-IB** Hewlett-Packard Interface Bus. A parallel interface that allows "daisy chaining" of more than one device to a port on a computer or instrument. Interface protocol is defined in IEEE 488.2; equivalent to the industry standard GPIB.

**HTTP** HyperText Transfer Protocol: Used to carry World Wide Web (WWW) traffic.

**Hue** The dimension of color referred to a scale of perceptions ranging from red through yellow, green, and blue, and back to red. A particular gradation of color, tint, shade.

---

|

**I/O** Input/Output

**I/O Path** Input/Output Path

**IEEE** Institute of Electrical and Electronic Engineers

**IF** Intermediate Frequency: the frequency at which a signal is processed after mixing.

**Impedance** The ratio of voltage to current at a port of a circuit, expressed in ohms.

**Initialize** The process that assigns information locations to a disk to prepare the magnetic media to accept files.

**Input** A path intended for putting a signal into an instrument.

Most network analyzers have either 3 (labeled A, B, and R) or 4 inputs (labeled A, B, R1, and R2). Inputs are not the same as channels.

**Input Attenuator** An attenuator between the input connector and the first mixer of a spectrum analyzer (also called an RF attenuator). The input attenuator is used to adjust the signal level incident to the first mixer, and to prevent gain compression due to high-level or broadband signals. It is also used to set the dynamic range by controlling the degree of internally-generated distortion. For some analyzers, changing the input attenuator settings changes the vertical position of the signal on the display, which then changes the reference level accordingly. In Agilent microprocessor-controlled analyzers, the IF gain is changed to compensate for changes in input attenuator settings. Because of this, the signals remain stationary on the display, and the reference level is not changed.

**Insertion Loss** The difference between the power measured before and after the insertion of a device. The attenuation between the input and output of a device.

**Intensity** Brightness; emitting or reflecting light; luminosity.

**Interface** A connection that allows a common communication link between two or more instruments.

**Intermodulation Distortion** Undesired frequency components resulting from the interaction of two or more spectral components passing through a device having nonlinear behavior, such as a mixer or an amplifier. The undesired components are related to the fundamental components by sums and differences of the fundamentals and various harmonics. The algorithm is:  $f_1 \pm f_2$ ,  $2xf_1 \pm f_2$ ,  $2xf_2 \pm f_1$ ,  $3xf_1 \pm 2xf_2$ , and so on.

**Internet** The connection of two or more distinct networks. Often a gateway or router is used to make the connection.

**Interpolate** To determine a value of a signal between two adjacent points by a procedure or algorithm.

**IP** Internet Protocol

**IP Address** Internet protocol address: a unique number that is assigned to each device which is to be connected to a TCP/IP network. Before using an analyzer on a network, your network administrator will need to assign an IP address. An IP address consists of a 32-bit value presented in decimal dot notation: 4 octets (bytes) separated by a dot.

**ISDN** Integrated Services Digital Network: A standard digital service capability that features one or more circuit-switched communication channels capable of carrying digital voice, data, or image signals, a packet-switched

channel for out-of-band signaling and control. In addition, ISDN provides a collection of standard and optional features that support information productivity for the user, providing higher-speed Internet access than analog systems.

**ISO** International Standards Organization

**Isolation** A specification or measure of the immunity that one signal has to being affected by another adjacent signal. The occurrence is known as crosstalk.

**Isolator** An RF device used for providing isolation between paths and components. Made from a 3-port circulator, the third port being terminated in a 50ohm load.

---

## J

---

## K

**Kilo** Prefix for one thousand.

**KB** Kilobyte

**Kb/s** Kilobytes per second

---

## L

**LAN** Local Area Network

**LANS** Local Area Network System

**LCD** Liquid Crystal Display

**LED** Light Emitting Diode

**LIF** Logical Interchange Format (used for older HP disk drives/computers)

**Limit Lines** Lines input by the user that overlay the analyzer's measurement data to allow automatic detection of data that is out of the acceptable range. Pass/Fail annotation, audio alarms, or electronic output can be triggered to notify the operator or on-line computer program of the over-limit condition.

**Limit-Line File** The user-memory file that contains the limit-line table entries.

**Limit-Line Table** The line segments of a limit line are stored in the limit-line table. The table can be recalled to edit the line segments, then restored in the limit-line file.

**Linear Device** A device in which the output is continuously proportional to the input.

**LO** Local Oscillator. In a superheterodyne system, the LO is mixed with the received signal to produce a sum or difference equal to the intermediate frequency (IF) of the receiver.

**LO Feedthrough** The response that in a superheterodyne system when the first local oscillator frequency is equal to the first IF.

**Load** A one port microwave device used to terminate a path in its characteristic impedance.

**Load Match** A measure of how close the device's terminating load impedance is to the ideal transmission line impedance. Match is usually measured as return loss or standing wave ratio (SWR) of the load.

**Local Lock Out** A condition or command that prevents analyzer front-panel entries (and disables the Local key).

**Local Operation** To operate manually from the front panel.

**Log** Logarithm

**Log Display** The display mode in which vertical deflection is a logarithmic function of the input signal amplitude. Log display is also called logarithmic display. The display calibration is set by selecting the value of the reference level position and scale factor in dB per division.

**LRM** Line-Reflect-Match. See [Calibration](#), [TRL](#), and [LRM](#).

---

## M

**Magnitude** The amplitude of a signal measured in its characteristic impedance without regard to phase. See also [Scalar](#).

**Marker** A graphical symbol along a display trace that is annotated with measurement characteristics of that specific data point.

**Marker Functions** Mathematical or statistical computation on the data of one or more markers to provide the operator more information. For example, the marker delta function calculates and displays the difference between two markers.

**Maximum Input Level** The maximum signal power that may be safely applied to the input of an analyzer. The maximum input level is typically 1 W (+30 dBm) for Agilent spectrum analyzers.

**MB** Megabyte

**Measurement Uncertainty** The quantified amount of error in a measurement situation. Calibrations are intended to reduce the amount of uncertainty. The following are sources of measurement errors that lead to uncertainty:

- Systematic errors (imperfections in calibration standards, connectors, cables, and instrumentation)
- Random errors (noise, connector repeatability)
- Drift (source and instrumentation)

**Mega** Prefix for one million.

**Memory** A storage medium, device, or recording medium into which data can be stored and held until some later time, and from which the entire original data may be retrieved.

**Memory Card** A small memory device shaped like a credit card that can store data or programs.

**Menu** The analyzer functions that appear on the display and are selected by pressing front panel keys. These selections may invoke a series of other related functions that establish groups called menus.

**MHz** Megahertz

**milli** Prefix for one-thousandth.

**Modem** Modulator/Demodulator

**Modulation** The process, or the result of the process, of varying a characteristic of a carrier signal with an information-bearing signal, causing the carrier to contain the information. See [AM](#) and [FM](#).

**Monitor** Any external display.

**Monochrome** Having only one color (chromaticity).

**ms** Millisecond

**mW** Milliwatt: one thousandth of a watt

**Multisync** A type of monitor that can synchronize its horizontal sweep to various frequencies within a specified range.

---

## N

**Narrowband** In network analysis, the frequency resolution of the analyzer's receiver that is sufficiently narrow to resolve the magnitude and phase characteristics of narrowband devices. The reduced receiver bandwidth usually decreases the noise floor of the receiver, providing more measurement amplitude range.

**Narrowband Device** A device whose transfer characteristics are intended to operate over a very narrow frequency range and are designed to provide well-defined amplitude responses in that range, such as a band pass filter.

**Network Analysis** The characterization of a device, circuit, or system derived by comparing a signal input going into the device to a signal or signals coming out from the device.

**NIST** National Institute of Standards and Technology

**Nit** The unit of luminance (photometric brightness) equal to one candela per square meter.

**Noise** Random variations of unwanted or disturbing energy in a communications system from man-made and natural sources that affects or distorts the information carried by the signal. See also [Signal-to-Noise Ratio](#).

**Noise Figure (F)**: For a two-port device, a measure of how the noise generated inside the device degrades the signal-to-noise ratio of a signal passing through the device at 290 degrees, usually expressed in dB.

**Noise Floor** The analyzer's internal displayed noise. The noise level often limits how small a signal magnitude can be measured. In network analysis, noise floor is measured with the test ports terminated in loads, full two-port error correction, 10 Hz IF bandwidth, maximum test port power, and no averaging during the test.

**Non-Insertable Devices** In measurement calibration, a device that cannot be substituted for a [Zero-Length Through Path](#). It has the same type and sex connectors on each port, or a different type of connector on each port.

**Nonvolatile Memory** Memory data that is retained in the absence of an ac power source. This memory is typically retained with a battery. Refer also to battery-backed RAM.

**Normalize** To subtract one trace from another to eliminate calibration data errors or to obtain relative information.

---

## O

**Offset** To move or set off a determined amount. Used in instruments for offsetting frequencies, limits, delay, loss, impedance, etc.

**Output Attenuation** The ability to attenuate the signal, the source, in order to control its power level.

---

## P

**PC** Personal Computer

**PDF** Portable Document Format (used on the Web)

**Parser, Command** Reads program messages from the input queue of a device in the order they were received from the controller. The parser determines what actions the analyzer should take. One of the most important functions of the command parser is to determine the position of a program message in the analyzer SCPI command tree. When the command parser is reset, the next element it receives is expected to arise from the base of the analyzer command tree.

**Peak Search** A function on an analyzer that searches for the largest response and places a marker on it.

**Phase** The fractional part of a cycle through which an oscillation has advanced, measured from an arbitrary starting point; usually measured in radians or degrees. In network analysis, the phase response of the device under test is the change in phase as a function of frequency between the input stimulus and the measured response.

**Port** The physical input or output connection of an instrument or device.

**Port Extension** Redefining the reference plane to other than that established at calibration. A new reference plane is defined in seconds of delay from the test set port.

**Positive Peak** The maximum, instantaneous value of an incoming signal.

**Postscript (.ps files)** Stores bitmapped graphics files in an encapsulated format for direct use by postscript printers.

**Power, Max Input** The upper limit to input power for which the specifications apply. Some specifications may have different levels of maximum inputs. For example, compression power maximum is usually higher than the harmonic distortion maximum.

**Power, Safe Input** The input power, usually in dBm, allowed without damaging the instrument.

**Preset** A pre-defined instrument state (that also runs an analyzer self-test). The action of pushing the Preset key.

**Protocol** A set of conventions that specify how information will be formatted and transmitted on a network, and how machines on a network will communicate.

---

## Q

**Q or Q Factor** The ratio of energy stored to energy lost in a resonant circuit. High Q indicates a sharp resonance response over frequency.

**Query** Any analyzer programming command having the distinct function of returning a response. These commands may end with a question mark (?). Queried commands return information to the computer.

---

## R

**r + jx** Expression for complex impedance, where r represents the resistive portion and x represents the reactive portion.

**R Channel** Reference Channel

**RAM** Random Access Memory, or read-write memory: A storage area allowing access to any of its storage locations. Data can be written to or retrieved from RAM, but data storage is only temporary. When the power is removed, the information disappears. User-generated information appearing on a display is RAM data.

**ROM** Read Only Memory: A storage area that can be read only; it cannot be written to or altered by the user. In instruments, the storage area that contains the "brains" or operational programming; the firmware.

**Receiver** A circuit or system designed for the reception and/or measurement of signals in a specified frequency spectrum.

**Receiver Dynamic Range** See [Dynamic Range](#).

**Reference Level** An instrument function that allows the user to set the amplitude value at the reference position. On network analyzers, the reference position is also selectable. On some spectrum analyzers, the reference position is fixed at the top of the display.

**Reference Plane** The electrical location at which a network analyzer assumes the system connectors and fixturing ends and the DUT begins. The reference plane is set by using calibration standards with known electrical length. The closer the reference plane is to the device under test (DUT), the better the characterization of the device because of the elimination of test system uncertainties.

**Reflection** The phenomenon in which a traveling wave strikes a discontinuity and returns to the original medium.

**Reflection Coefficient** The ratio of the reflected voltage to the incident voltage into a transmission line or circuit. If a transmission line is terminated in its characteristic impedance, the reflection coefficient is zero. If the line is shorted or open the coefficient is 1. See also [Return Loss](#) and [SWR](#).

**Reflection Measurements** Measurements that characterize the input and /or output behavior of the device under test (DUT). Measured as the ratio of the reflected signal to the incident signal as a function of frequency. Parameters are called return loss, reflection coefficient, impedance, and standing wave ratio (SWR), all as a function of frequency. See also [S-Parameters](#).

**Remote** A mode of operation where another device (or computer) controls an instrument via the HP-IB. In this mode, the instrument front panel keys are disabled. Front panel operation is called local operation.

**Remote Programming** The automatic operation of an instrument by a computer, usually through a HP-IB, LAN, or RS-232 link.

**Resolution** The ability of a receiver to resolve two signals.

**Resolution Bandwidth** The ability of a spectrum analyzer to display adjacent responses discretely (Hertz, Hertz decibel down). This term is used to identify the width of the resolution bandwidth filter of a spectrum analyzer at some level below the minimum insertion loss point (maximum deflection' point on the display). Typically, it is the 3 dB resolution bandwidth that is specified, but in some cases the 6 dB resolution bandwidth is specified.

**Return Loss** The amount of dB that the reflected signal is below the incident signal. If zero signal is reflected, the

impedance of the device is equal to the characteristic impedance of the transmission system, and return loss is infinite. If the entire incident signal is reflected, the return loss is zero. See also [S-Parameters](#), [Reflection Coefficient](#), and [SWR](#).

**Reverse Measurement** The measurement of a device from output to input.

**RF** Radio Frequency (from approximately 50 kHz to approximately 3 GHz). Usually referred to whenever a signal is radiated through the air.

**ROM** Read Only Memory

---

## S

**S/N** Signal-to-Noise Ratio

**Sampler** An electronic component that captures the signal level and phase across a known impedance at a uniform rate. In Network Analyzers, this sampling rate must be sufficiently high and precisely timed to make accurate measurements. Network analyzers typically have three or four samplers or mixers.

**Sampler Bounce** The leakage or crosstalk between a network analyzer's samplers. Delay in this crosstalk caused by leakage transmission propagation, give the interference its "bounce" appearance. Sampler bounce causes an increase in the noise level of the affected channel, reducing the sensitivity of the analyzer.

**Saturation** The degree of color purity, on a scale from white to pure color.

**Scalar** A quantity that has magnitude but no phase. A network analyzer capable of measuring only magnitude.

**Scale Factor** The display vertical axis calibration in terms of units per division.

**SCPI** Standard Commands for Programmable Instruments

**Screen** The physical surface of the CRT or flat panel upon which the measurement results, setup information, softkey definitions, and other instrument communication is presented.

**Self-Test** A group of tests performed at power-up (or at preset) that verify proper instrument operation.

**Sensitivity** The minimum input signal required to produce a specified output signal having a specified signal-to-noise ratio, or other specified criteria.

On a spectrum analyzer, the level of the smallest sinusoid that can be observed, usually under optimized conditions of minimum resolution bandwidth, 0 dB input attenuation, and minimum video bandwidth.

The normalized change in YIG component's center frequency resulting from a change in tuning coil current, specified in MHz/mA.

**Serial Prefix** The five-character prefix that begins an instrument serial number; used to represent versions of firmware or hardware changes that have occurred.

**Server** A device that is configured to provide a service to other devices on a network, such as shared access to a file system or printer.

**Signal-to-Noise Ratio** SNR: The ratio of the amplitude of the desired signal to the amplitude of noise signals, usually expressed in dB and in terms of peak values for impulse noise and root-mean-square values for random noise.

**Single Sweep Mode** The spectrum analyzer sweeps once when trigger conditions are met. Each sweep is initiated by pressing an appropriate front panel key, or by sending a programming command.

**Small Signal Gain Compression** A situation when the input signal's measured amplitude is less than its actual level due to overloading of the network analyzer's input mixer; the analyzer is operating nonlinearly. For broadband analyzer detectors, a signal other than the one under test can put the analyzer into this gain compressed mode, thereby making even lower level signals appear at a lower level than actual. The broadband mode measures all the power incident to the analyzer, not just the signals at the frequency of interest.

**Smith Chart** A graphical mapping of the complex reflection coefficient into normalized complex impedance. Circles on the chart represent constant resistance and radiating lines orthogonal to the circles represent constant reactance. The center of the chart represents the characteristic impedance of the transmission system. Any point

on the chart defines a single complex impedance. A line on the chart represents changing impedance over frequency.

**SOLT** Short-Open-Load-Through calibration. See also [Calibration, SOLT](#).

**Source** A device that supplies signal power; a sweep oscillator or synthesized sweeper.

**Source Amplitude Accuracy** The amplitude uncertainty, in dB, of the source power readout.

**Source Amplitude Flatness** The amplitude flatness, in dB, of the source power over the frequency range specified.

**Source Frequency Resolution** The smallest unit of frequency which can be set and/or measured, in Hz.

**Source Frequency Time Base Accuracy** A measure of the analyzer's frequency stability measured in parts per million (ppm. or 1 part in 10E6). For example, a stability of  $\pm 5.0$  ppm means that an analyzer will measure 1 MHz to an accuracy of  $\pm 5 \times 10^{-6} \times 10^6 \text{ Hz} = \pm 5 \text{ Hz}$ .

**Source Frequency Time Base Stability** A measure of the analyzer's time base accuracy over time and temperature. Typically the time base accuracy will be specified for 1 year. A typical temperature frequency stability is  $\pm 10$  ppm for 250 C  $\pm$  50 C.

**Source Harmonics** The level of harmonics generated by the analyzer's signal source, in dBc from the fundamental.

**Source Match** A measure of how close the signal source impedance is to the ideal transmission line impedance of the test system. Match is usually measured as return loss or standing wave ratio (SWR) of the source.

**Span** The stop frequency minus the start frequency. The span setting determines the horizontal-axis scale of the analyzer display.

**Span Accuracy** The uncertainty of the indicated frequency separation of any two signals on the display.

**S-Parameters (Scattering Parameters)** A convention used to characterize the way a device modifies signal flow using a network analyzer. A two port device has four S-parameters: forward transmission (S21), reverse transmission (S12), forward reflection (S11), and reverse reflection (S22).

**Stop/Start Frequency** Terms used in association with the stop and start points of the frequency measurement range. Together they determine the span of the measurement range.

**Storage States** The number of settings, programs, traces, and other parameters available to be saved, cataloged, and recalled at any one time.

**Storage, Disk** An internal or external digital storage disk for saving test data, instrument settings, IBASIC programs, and other measurement parameters. Storage formats include MS-DOS (R) and HPs standard LIF with binary, PCX, HP-GL, or ASCII data formats.

**Structural Return Loss** Poor return loss in cable due to a periodic fault such as a periodic dent caused by dropping the cable spool or by the cable pulling process during manufacture.

**Supplemental Characteristics** Typical but non-warranted performance parameters, denoted as "typical", "nominal" or "approximate".

**Sweep** The ability of the source to provide a specified signal level over a specified frequency range in a specified time period. Also see [Sweep Mode](#) and [Sweep Type](#).

In data processing mode, a series of consecutive data point measurements, taken over a sequence of stimulus values.

**Sweep Mode** The way in which a sweep is initiated or selected, e.g., single, continuous, alternate, or chopped.

**Sweep Type** The method of sweeping the source, e.g., linear, log, or frequency step.

**Sweeper** A signal source that outputs a signal that varies continuously in frequency.

**SWR** Standing Wave Ratio, calculated as  $(1 + \pi) / (1 - \pi)$  where  $\pi$  is the reflection coefficient.

**Sync** Synchronization, or Synchronized

**Syntax** The grammar rules that specify how commands must be structured for an operating system, programming language, or applications.



**System Dynamic Range** The difference between the maximum receiver input level and the receiver's noise floor. System dynamic range applies to transmission measurements only, since reflection measurements are limited by directivity.

---

## T

**T/R** See [Transmission/Reflection](#).

**Termination** A load connected to a transmission line or other device.

**Test Limit** The acceptable result levels for any given measurement.

**Test Port** See [Port](#).

**Test Set** The arrangement of hardware (switches, couplers, connectors and cables) that connect a test device input and output to the network analyzer's source and receiver to make s-parameter measurements.

**Third Order Intercept** TOI: The power input to a non-linear device that would cause third order distortion at the same power level. TOI is a measurement to determine the distortion characteristics of a mixer or receiver. The higher the value, the more immune the receiver to internal distortion.

**Thru** Through line: A calibration standard. See [Calibration](#), [SOLT](#).

**Tint** A shade of color; hue.

**Toggle** To switch states, usually to change a function from on to off, or off to on.

**TOM** Thru-Open-Match: A Rohde&Schwarz term to describe a calibration method.

**Trace** A series of data points containing frequency and response information. The series of data points is often called an array. The number of traces is specific to the instrument.

**Tracking** The ability of the analyzer's receiver to tune to the source frequency over the measurement frequency range. Poor tracking results in amplitude and phase errors due to the receiver IF circuits attenuating and delaying the device under test output.

**Transfer Function** The ratio of the output signal to the stimulus signal, both as a function of frequency.

**Transmission** See [Transmission Measurements](#).

**Transmission Intermodulation Spurious** A measure of the capability of the transmitter to inhibit the generation of intermodulation distortion products. Intermodulation spurious is sometimes called intermodulation attenuation.

**Transmission Measurements** The characterization of the transfer function of a device, that is, the ratio of the output signal to the incident signal. Most common measurements include gain, insertion loss, transmission coefficient, insertion phase, and group delay, all measured over frequency. See also [S-Parameters](#).

**Transmission/Reflection (T/R)** Refers to the suite of measurements made by a scalar or vector network analyzer to characterize a device's behavior over frequency. See also [S-Parameters](#).

**Transparent** Something that is not visible to the user. Usually a procedure that occurs without the user's initiation or knowledge.

**Trigger** A signal that causes the instrument to make a measurement. The user can select several options for triggering, such as manual, continuous, or external (for synchronizing measurements to an external source).

**TRL** Through-Reflect-Line. See [Calibration](#), [TRL](#) and [LRM](#).

**TTL** Transistor-Transistor Logic

**Two-Port Error Correction** See [Error Correction](#), [12-Term](#).

---

## U

**Uncorrected** Measurements made without performing error correction.

**Uncoupled Channels** Stimulus or receiver settings allowed to be set independently for each channel.

**UNI** User-Network Interface: The point at which users connect to the network.

**Units** Dimensions on the measured quantities. Units usually refer to amplitude quantities because they can be changed. In analyzers with microprocessors, available units are dBm (dB relative to 1 mW dissipated in the nominal input impedance), dBmV (dB relative to 1 mV), dBW (dB relative to 1 W), V (volts), W (watts).

---

## V

**Variable** A symbol, the value of which changes either from one iteration of a program to the next, or within each iteration of a program.

**Vector** A quantity that has both magnitude and phase.

A network analyzer capable of measuring both magnitude and phase.

**VEE** Visual Engineering Environment (Agilent software product)

**Velocity Factor** A numerical value related the speed of energy through transmission lines with different dielectrics (.66 for polyethylene). Used in making time domain measurements.

**Vertical Resolution** The degree to which an instrument can differentiate amplitude between two signals.

**Video** An electrical signal containing timing, intensity, and often color information that, when displayed, gives a visual image.

**Video Bandwidth** In spectrum analyzers, the cutoff frequency (3 dB point) of an adjustable low-pass filter in the video circuit. When the video bandwidth is equal to or less than the resolution bandwidth, the video circuit cannot fully respond to the more rapid fluctuations of the output of the envelope detector. The result is a smoothing of the trace, or a reduction in the peak-to-peak excursion, of broadband signals such as noise and pulsed RF when viewed in broadband mode. The degree of averaging or smoothing is a function of the ratio of the video bandwidth to the resolution bandwidth.

**Video Filter** In spectrum analyzers, a post-detection, low-pass filter that determines the bandwidth of the video amplifier. It is used to average or smooth a trace. Refer also to [Video Bandwidth](#).

**VNA** Vector Network Analyzer

---

## W

**Waveform** A representation of a signal plotting amplitude versus time.

**Wireless** A term that refers to a broad range of technologies that provide mobile communications for home or office, and "in-building wireless" for extended mobility around the work area, campus, or business complex. It is also used to mean "cellular" for in-or out-of-building mobility services.

**WWW** World Wide Web

---

## X

---


## Y


---


## Z

**Zero-Length Through Path** In a measurement calibration, when the two test cables mate together directly without using adapters or a thru-line. See also [Non-Insertable Devices](#).



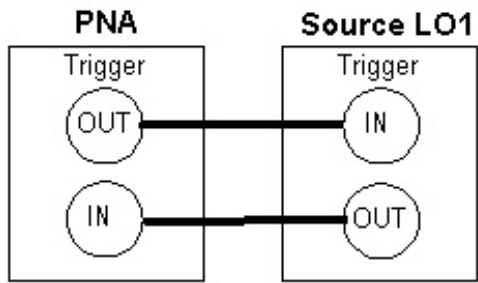

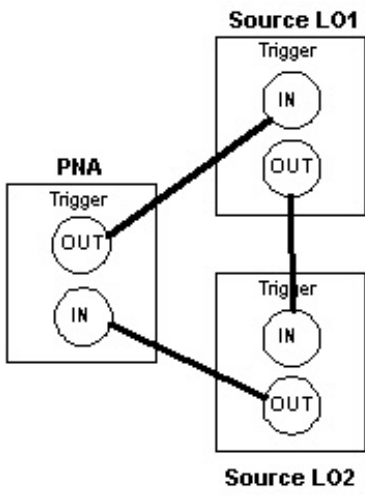





**Agilent Technologies**



Quick Start



Setup



Speed/Accuracy



Calibrate




Analyze Data



Print / Save



Tutorials



Programming

### CRITICAL NOTES ABOUT YOUR HARD DRIVE

What's New


Frequency Offset

Pulsed App / IF Access


Product Support / Specs

PNA Connectivity


PNA Help / Rev

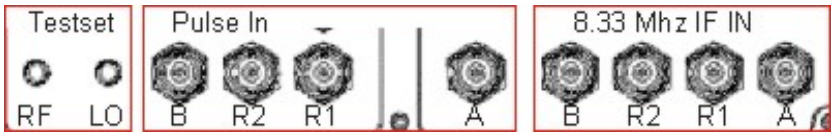





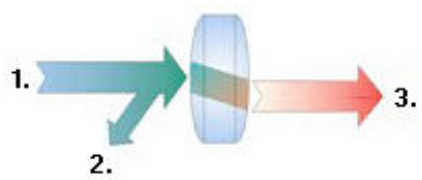





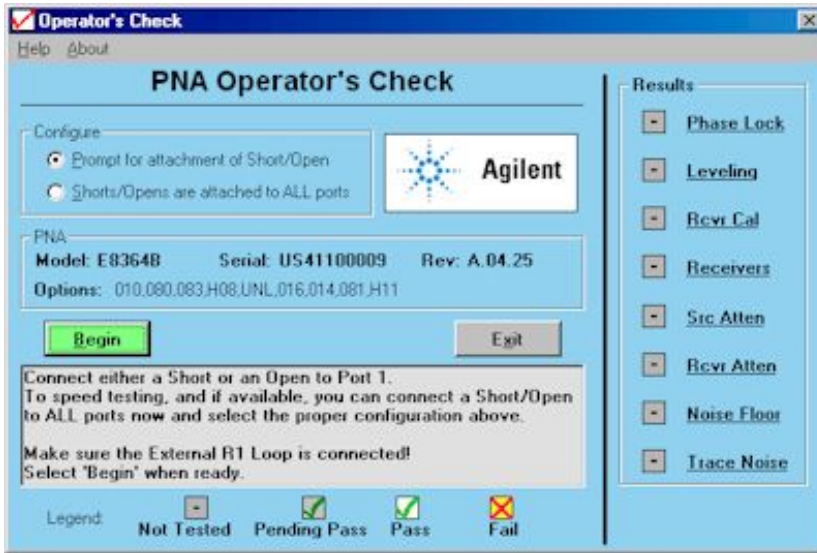


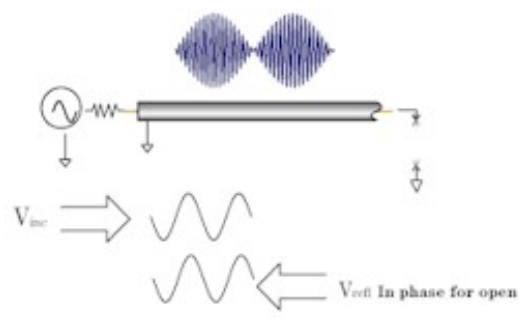

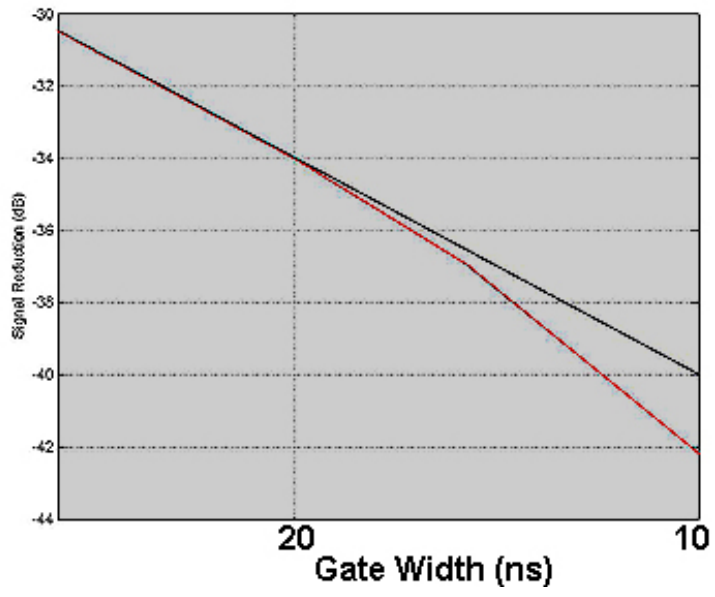


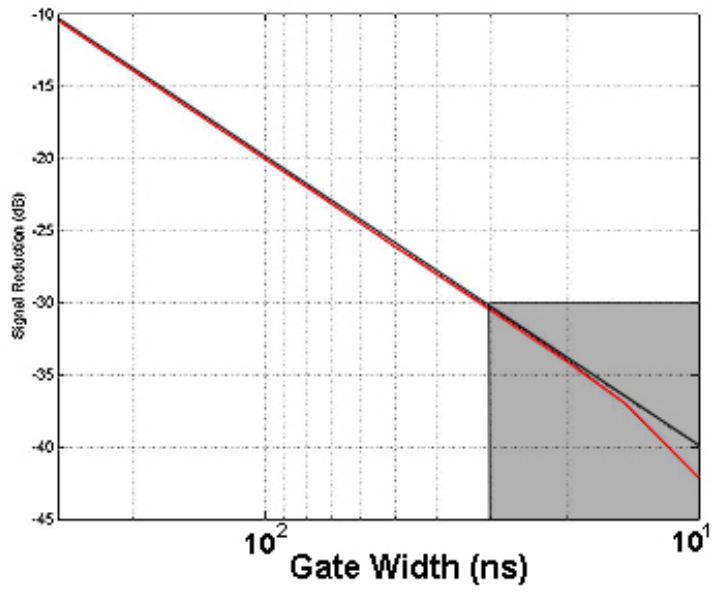


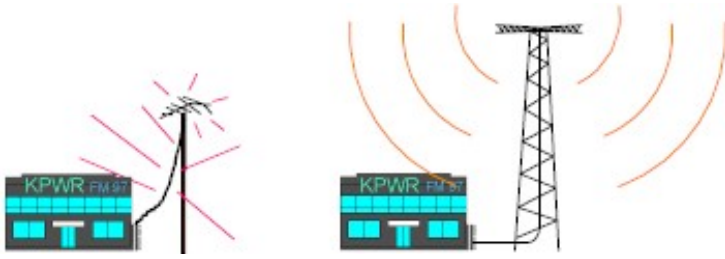


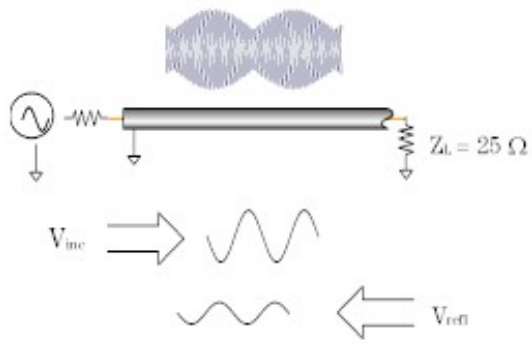



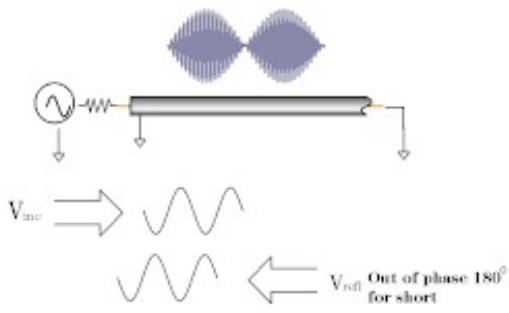

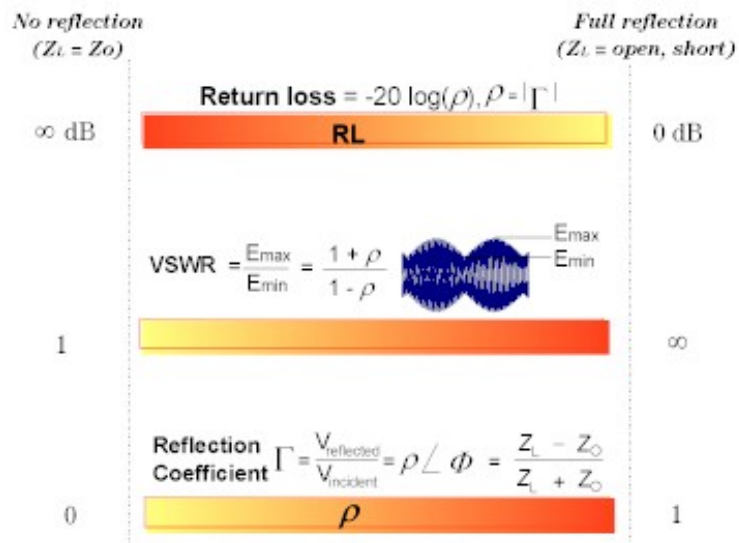

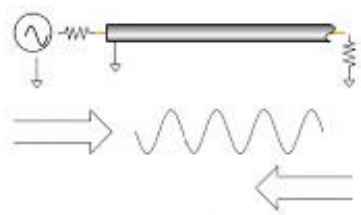

## Frequency Offset Measurements

---

Frequency Offset measurements require the PNA source to tune to a different frequency than the PNA receiver. This capability is offered as an [option on some PNA models](#).

To view the options that are installed on your PNA, click **Help** then **About Network Analyzer**

**[Frequency Offset](#)** (Option 080) - Allows basic frequency converter measurements

**[Frequency Converter Application](#)** (Option 083) - Allows you to easily make extremely accurate scalar and phase frequency converter measurements. [See Known Issues](#).

**[Tutorials](#)** - Learn how to make specific Frequency Conversion Device Measurements

## 3.5" Floppy Disk Drive

[Return to Front Panel](#)

---



Installs files on the analyzer hard drive or stores data files from the analyzer. Access the disk drive by using Windows Explorer.

- Unformatted Data Capacity: 2MB
- Compatible with: High Density (2HD), and Normal Density (2DD)
- Transfer Rate: 500 kbits/second

## Arrange Key

---



Allows you to choose from four window arrangements: Overlay, Stack 2, Split 3, Quad 4.

[Learn More about Arranging the Display](#)

## Average Key

---

Allows you to apply measurement averages which reduces noise. The analyzer performs a complex exponential average of a number of sweeps that you specify.

[Learn more about Averaging](#)

## Calibration Key

---

Initiates a measurement calibration. The Calibration Wizard appears if you press Menu/Dialog, Cal. Otherwise, pressing the Cal key makes the calibration active entry toolbar appear.

[Learn more about Calibration](#)



## Cancel Key

---

Closes a dialog box.

## Channel Key

---

Allows you to select an active channel, or delete a channel. A channel must be active to modify any channel settings.

[Learn more about Channels](#)

Click a key to learn its function:



These keys allow you to:

- Configure a channel with various stimulus settings.
- Perform a measurement calibration.

[Learn more about Channels](#)

Click a key to learn its function:



These keys allow you to:

- Issue commands in a dialog box.
- Display menus or dialog boxes.
- Launch the analyzer Help.

## Decimal Point Key

---

Enters a decimal point to designate fractions of a whole number.

Click a key to learn its function:



These keys allow you to:

- Manage and create traces and windows.
- Quickly configure a set of measurements.
- Arrange the display of current measurements.


[Learn more about the Display](#)

## Enter Key

---

Enters the values that you select for the measurement settings.

Click a key to learn its function:

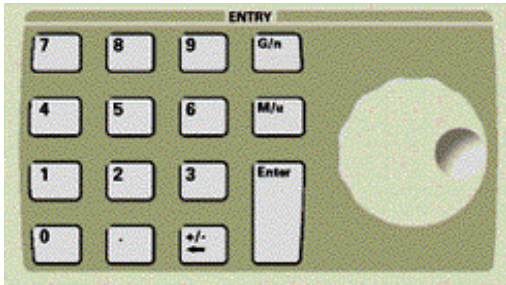

These keys allow you to enter values for measurement settings.



## Format Key

---

Allows you to select the format the analyzer uses to display the measurement data.

[Learn more about Data Format](#)

## Front-Panel Jumpers

---

### [PNAs with a Configurable Test Set](#)

#### [E835xA Standard PNA](#)

What is a [configurable test set](#)?

---

**Note:** Standard analyzers, with the exception of the E835xA and N5250A, do not have front-panel jumpers.

---

### Front-Panel Jumpers on PNAs with a Configurable Test Set

Configuration graphics and specifications:

[E835xA, Option 015](#)

[E880xA, Option 014](#)

[N338xA, Option 014](#)

[E8361A Option 014](#)

[E8362A/B, 63A/B, 64A/B Option 014](#)

[N5230A, Option 225, or 425, or 525 \(2-Port Models\)](#)

[N5230A, Option 245 \(4-Port Model\)](#)

[N5250A \(no specs available\)](#)

Use the front-panel jumpers of your PNA's configurable test set to do the following.

- Test high power devices by adding your own external components in the measurement path.
- Configure signal path for up to 143 dB dynamic range at the test port with full 12-port error correction. To do so, use segment sweep mode and simply reverse the coupler using the front-panel jumpers for increased dynamic range in one direction .

### Front-Panel Jumpers on the E835xA Standard PNA

Configuration graphics and specifications:

[E835xA](#)

Use the E835xA standard front-panel jumpers to do the following:

- Test high power devices by adding your own external components in the measurement path.
- Bypass the test-port couplers and apply signals directly into the receivers for improved signal-to-noise ratio. Achieve up to 143 dB dynamic range with response calibration using segment sweep mode.

For more information on front-panel jumpers, see:


- [High-power amplifier measurements](#)
- [Dynamic range measurements](#)
- [Analyzer options](#)

- Arbitrary Ratio

## Help Key

---

Launches the analyzer Help (embedded documentation).



These connectors provide direct access to the PNA source and receivers. This allows you to make high-power measurements and improve dynamic range. Front panel jumpers are OPTIONAL; not all PNA's have this capability.

Learn about the jumpers on **YOUR** PNA.

## Limit Table Key

---

Displays the table of values that allow you to create pass / fail testing based on these limit segments.

## Macro / Local Key

---

When the analyzer is being controlled through automation, pressing this key allows the analyzer to respond to front panel key presses.

When the analyzer is in normal operation, pressing this key accesses a set of user macros that are in the form of executable files. You can title and store up to 12 macros. When you repeatedly press this key, the titles in the active entry toolbar rotate through three sets of four titles.

---

**Note:** You must have the applications installed on the analyzer hard disk that are necessary to run the executable files in the set of macros.

---

## Math / Memory Key

---

Allows you to select math and memory functions that the analyzer performs on the measurement data.



## Measure Key

---

Allows you to select an S-parameter measurement. Through the dialog box you can also select an arbitrary ratio, or unratiod power measurement.

## Measure Setups Key

---

Allows you choose from four pre-configured measurement setups.

## Menu / Dialog Key

---

Allows you to browse the menus with the Navigation keys. Also allows you to display dialog boxes by pressing Menu/Dialog and then a key in the Channel, Trace, or Utility blocks.

## Restore Up/Down Key

---



Changes the selected window to the full measurement screen size and then restores it to the previous window size.

Restores the PNA application if minimized.

## Marker Key

---

Allows you to activate a marker and set the value. Markers provide numerical readout of measured data.

## Marker Function Key

---

Allows you to change measurement settings, based on the location of an active marker. If there is no marker displayed, this key will activate a marker.

## **Marker Search Key**

---

Provides access to the marker search functions. If there is no marker displayed, this key will activate a marker.


## Marker Table Key

---

Displays the table of values that allow you to view the data readout for all of the markers on the active trace.



Click a key to learn its function:

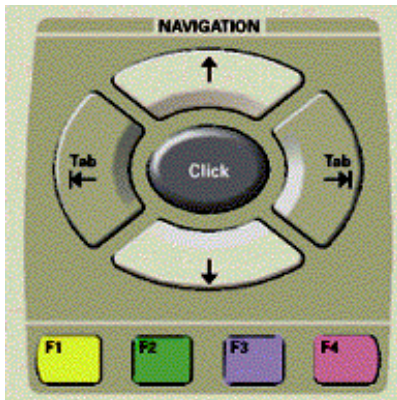

These keys allow you to navigate through menus and dialog boxes and select choices from the active entry toolbar.

**Left /  
Right**

Moves left and right through menus

Moves tab-left and tab-right within dialog boxes

**Up /  
Down**

Moves up and down through menus

Behaves as follows in a dialog box:

- Modifies a numeric value
- Moves through items in a drop-down list
- Moves through options buttons in a group of option buttons

**Click**

Makes a selection just like a mouse click

**F1...F4  
Keys**

Selects choices from the active entry toolbar. The color of the key corresponds to the active entry toolbar choice. [Learn more about Active Entry Keys.](#)

## Numeric Keys

---

Selects values for measurement settings, then press **Enter** or **G/n** or **M/u** to complete the selection.

## **OK Key**

---

Closes a dialog box and enters any values made in the dialog box.



Toggles the analyzer between the On and Hibernate conditions.

- For the On condition the button is green.
- For the Hibernate condition the button is an orange-yellow light.
- To switch off the analyzer, press the power button and the instrument saves the states of all the programs running and switches off the power.
- When you press the button again, the instrument loads the states that were saved at the time the power was switched off.

This switch is not connected to the power supply.

## Plus - Minus - Backspace Key

---

- Toggles between a positive and negative value entry if it is the first key pressed in the entry.
- Backs up the cursor and deletes any previous selection.

## Power Key

---

Allows you to specify the source power level.

## **Preset Key**

---


Changes the analyzer to its preset (default) conditions.

## **Print Key**

---

Initiates a print function, allowing you to select the print conditions and printer.





The 3-pin (m) connectors supply power for active probes.

- Top Pin: Ground
- Left Pin: +15 VDC  $\pm 2\%$ , 400 mA maximum; protected by PTC @0.5A
- Right Pin: -12.6 VDC  $\pm 5\%$ , 300 mA maximum; protected by PTC @0.5A

(PTC=slow acting, automatically resettable fuse)

## Recall Key

---

Allows you to recall a file that contains an instrument state, measurement calibration, and measurement data.

## Front Panel Knob

---

Rotates to increase or decrease the value of the active entry.

## Save Key

---


Allows you to save instrument states, calibration data, and measurement data to a file.

## Scale Key

---

Allows you to specify the value the analyzer uses to scale the displayed measurement response. You can also let the analyzer automatically set the Y axis scales to fit the entire measurement trace on the screen.

Click on an area to learn its function.

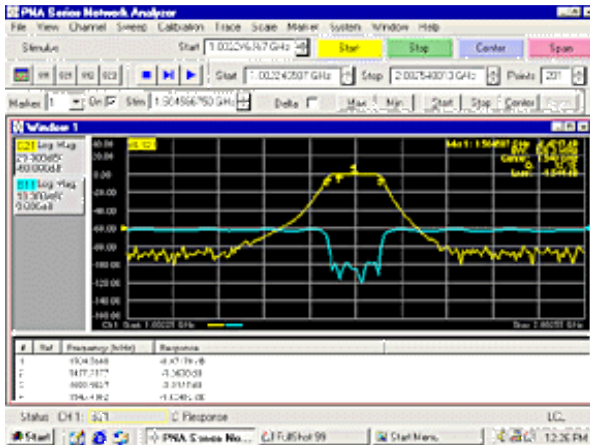

This display screen has the following characteristics:

- Active Matrix (TFT), 8.4 inches, LCD
- Resolution: 640 x 480 Resolution
- Vertical Refresh Rate: 59.83 Hz
- Horizontal Refresh Rate: 31.41 kHz
- Brightness: >250 NIT

[Learn to Configure the Screen](#)

## Stop / Span Key

---

Allows you to enter a value for the stop or span of the measurement range.

## Start / Center Key

---

Allows you to enter a value for the start or center of a measurement range.



## **Sweep Setup Key**


---

Allows you to define how the analyzer source provides a stimulus to a device under test.

## **Sweep Type Key**

---

Allows you to select the way the analyzer source sweeps, and the properties associated with the sweep.

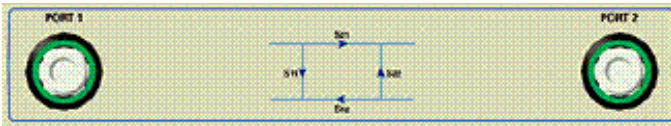

See [PNA Configurations](#) for a list of test port connector types.

PNA test ports internally switch between source and receiver allowing measurement of your device in two directions.

Two different lighting methods are used to indicate the source and receiver port:

For 9 GHz and below PNA models (shown above):

- A **green** light indicates the **source** port.
- An **orange** light indicates the **receiver** port.

All other PNA models:

- An illuminated image next to the test port indicates the source.

---

**Note:** The following PNA model has three test ports: N3381A, N3382A, N3383A.

---

See [Input Damage Levels](#)

## Trace Key

---

First press brings up the Trace Active Toolbar. Subsequent presses allow you to cycle through the measurement traces in a window, making each trace active in turn. You can make modifications only to active functions. This key also allows you to create or delete traces, using the function keys.

Click a key to learn its function:



These keys allow you to:

- Configure a measurement type
- Extract data from the results

## Trigger Key


---

Allows you to specify how the start of the measurement sweep is initiated.

## Units Keys

---

Completes the value selection, assigning a unit of measurement. Then press **Enter** to complete the value entry.



This Type A Universal Serial Bus (USB) connector allows you to connect a keyboard, mouse, ECAL module, or other USB device.

- Contact 1: Vcc; 4.75 to 5.25 VDC, 500 mA maximum. Protected with an automatically-resettable 1A fuse.
- Contact 2: -Data
- Contact 3: +Data
- Contact 4: Ground

[See USB limitations.](#)



Click a key to learn its function:



These keys allow you to:

- Print measurement results.
- Save or recall the following:
  - Instrument states
  - Measurement Calibrations
  - Measurement Data
- Run macros.
- Manipulate the window size.
- Preset the analyzer.

## Window Key

---

First press brings up the Window Active Toolbar, where you can create, select, and delete windows, using the function keys.

Subsequent presses of this key cycle through the windows that are currently set up, making each window active in turn. You can make size modifications only to an active window. A window must also be active to cycle through the traces in the window.

## IF Access Overview

---

[About the H11 Option](#)

[Pulsed Application \(H08 Option\)](#)

[External Millimeter Module Configuration](#)

[SCPI Commands](#)

[GOM Commands](#)

[Option H11 Verification](#)

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

**Click a box or circle to view details:**

See [8510 data processing mode](#).

---

**Measurement** - PNA receivers gather complex trace data which is ratioed if required by the parameter, such as S11 or A/B. Otherwise it is raw receiver data, such as A or B. See [Measurement Parameters](#).

---

**Averaging** - If turned ON, data is averaged with specified number of measurement traces. See [Averaging](#).

**Data Access Point 0** - Get or Put **RAW MEASUREMENT data** using:

**SCPI** - [Calc:Data](#) SDATA (Correction OFF) or [Calc:RDATA](#)

**COM** - [getData](#) and [putDataComplex](#) - naRawData (0)

See [Formatting Note](#)

---

**Acquired Cal Data** - Calibration standards are measured. When the calibration is complete, complex data is stored in a Cal Set.

**Data Access Point 6** - Get or Put **RAW CAL ACQUISITION data** using:

**SCPI** - None

**COM** - [getStandardComplex](#) and [putStandardComplex](#)

---

**Calculate Error Terms** - Error terms are calculated from Acquisition data using formulas which are appropriate for the selected calibration method. Complex error terms are stored in a Cal Set. See [Systematic Errors](#).

**Data Access Point 7** - Get or Put **ERROR TERM data** using:

**SCPI** - [Calc:Data Error Terms](#)

**COM** - [Error Term commands](#)

---

**Apply Error Terms** - If error correction is ON, error terms are applied to the raw measurement data. Otherwise, this data is identical to Raw Measurement Data.

**Data Access Point 1** - Get or Put **CORRECTED data** using:

**SCPI** - [Calc:Data](#) SDATA (Correction ON)

**COM** - [getData](#) and [putDataComplex](#) - naCorrectedData (1)

See [Formatting Note](#)

---

**Normalization** - If performing Receiver power correction, "Divisor" (Data Access Point 5) correction data is applied to the measurement. See [Receiver power calibration](#)

**Data Access Point 5** - Get or Put **DIVISOR (POWER CAL) data** using:

**SCPI** - [Calc:Data](#) SDIV

**COM** - [getData](#) and [putDataComplex](#) - naDivisor (5)

See [Formatting Note](#)

---

**Trace Math** - If turned ON, memory data is combined with measurement data using the selected math function. Available functions are: Data+Mem, Data-Mem, Data\*Mem, and Data/Mem. See [Math Operations](#).

---

**Memory** - Data that is stored as a result of a **Data-To-Memory** operation. Each measurement can have one memory trace. The memory data parallels the measurement data through the remaining processing blocks. For example, turning smoothing ON will smooth both the measurement and memory traces.

**Data Access Point 3** - Get or Put **MEMORY data** using:

**SCPI** - [Calc:Data SMEM](#)

**COM** - [getData](#) and [putDataComplex](#) - naRawMemory (3)

See [Formatting Note](#)

---

**Gating** - If turned ON, Filter Gating is applied to the measurement data. Gating "virtually" removes undesired responses from selected regions of the trace. See [Gating](#).

---

**Phase Correction** - If turned ON, applies electrical delay, phase offset, and port extensions. These are all separate features that are controlled individually. See [Phase Measurement Accuracy](#).

---

**Magnitude Offset** - If entered, offset values are applied to the magnitude (real) portion of the data. See [Magnitude Offset](#).

---

**Time Domain** - If turned ON, transforms the data from the frequency domain to the time domain. See [Time Domain](#)

---

**Formatter** - Complex data is converted into scalar data formats for screen display and remote access. For smoothed data, request the data in the same format as the displayed data. See [Data Format](#)

---

**Smoother** - If turned ON, removes discontinuities in the measurement and memory trace. See [Smoothing](#).

---

**Display** - Displays the processed measurement, memory data, or both, in the format of your choice.

**Data Access Point 2** - Get or Put **MEAS RESULT data** using:

**SCPI** - [Calc:Data FDATA](#)

**COM** - [getData](#) and [putDataComplex](#) - naMeasResult (2)

**Data Access Point 4** - Get or Put **MEMORY RESULT data** using:

**SCPI** - [Calc:Data FMEM](#)

**COM** - [getData](#) and [putDataComplex](#) - naMemoryResult (4)

---

**Formatting Note:**


**COM** - [getData](#) allows you to request data from locations 0 to 5 in a format other than the displayed format.

SMOOTHED data is only attainable from locations 2 & 4, and only when you request data in the same format as the displayed format.

**SCPI** - you can only request data in the displayed format.

---

New See [Calibrating the PNA Using SCPI](#)

| <b>Perform an Unguided Calibration</b>                                                                                 |                                           |                                         |
|------------------------------------------------------------------------------------------------------------------------|-------------------------------------------|-----------------------------------------|
| Launch Cal Wizard                                                                                                      | <u>SYST:CORR:WIZard</u>                   | <u>app.LaunchCalWizard</u>              |
| Set Cal Type                                                                                                           | <u>SENS:CORR:COLL:METHod</u>              | <u>cal.SetCallInfo</u>                  |
| Select a Cal Kit                                                                                                       | <u>SENS:CORR:COLLect:CKIT</u>             | <u>app.CalKitType</u>                   |
| Get a Handle to the Active Cal Kit                                                                                     |                                           | <u>app.ActiveCalKit</u>                 |
| Simultaneous 2-Port Calibration                                                                                        | <u>SENS:CORR:TSTandards</u>               | <u>cal.Simultaneous2PortAcquisition</u> |
| Acquisition Direction                                                                                                  | <u>SENS:CORR:SFORward</u>                 | <u>cal.AcquisitionDirection</u>         |
| Measure a Standard                                                                                                     | <u>SENS:CORR:COLLect</u>                  | <u>cal.AcquireCalStandard</u>           |
| Calculate Errors                                                                                                       | <u>SENS:CORR:COLL:SAVE</u>                | <u>cal.CalculateErrorCoefficients</u>   |
| Do Isolation                                                                                                           | <u>SENS:CORR:COLLect</u>                  | <u>cal.AcquireCalStandard</u>           |
| <b>Perform a Guided Cal</b>                                                                                            |                                           |                                         |
| Initiate a Guided Cal                                                                                                  | <u>SENS:CORR:COLL:GUID:INIT</u>           | <u>Initialize</u>                       |
| List valid Connector Types for a Port                                                                                  | <u>SENS:CORR:COLL:GUID:CONN:CAT?</u>      | <u>ValidConnectorType</u>               |
| List valid Cal Kits for a Port                                                                                         | <u>SENS:CORR:COLL:GUID:CKIT:PORT:CAT?</u> | <u>CompatibleCalKits</u>                |
| Select a Connector Type                                                                                                | <u>SENS:CORR:COLL:GUID:CONN:PORT</u>      | <u>ConnectorType</u>                    |
| Select a Cal Kit                                                                                                       | <u>SENS:CORR:COLL:GUID:CKIT:PORT</u>      | <u>CalKitType</u>                       |
| Set Thru Method                                                                                                        | <u>SENS:CORR:COLL:GUID:METHod</u>         | <u>ThruCalMethod</u>                    |
| Set Thru Port Pairs                                                                                                    | <u>SENS:CORR:COLL:GUID:THRU:PORT</u>      | <u>ThruPortList</u>                     |
| Return Number of Steps in a Cal                                                                                        | <u>SENS:CORR:COLL:GUID:STEPS?</u>         | <u>GenerateSteps</u>                    |
|  Return a Description of a Cal Step | <u>SENS:CORR:COLL:GUID:DESC?</u>          | <u>GetStepDescription</u>               |
| Measure a Cal Standard in a Guided Cal                                                                                 | <u>SENS:CORR:COLL:GUID:ACQuire</u>        | <u>AcquireCalStandard</u>               |
| Calculate Error Terms from a Guided Cal                                                                                | <u>SENS:CORR:COLL:GUID:SAVE</u>           | <u>GenerateErrorTerms</u>               |
| <b>Perform an ECAL</b>                                                                                                 |                                           |                                         |
| Specify Module and Characterization                                                                                    | <u>SENS:CORR:COLL:ACQ</u>                 | <u>cal.ECALCharacterizationEx</u>       |
| Do ECAL 1-Port                                                                                                         | <u>SENS:CORR:COLL:CKIT 99</u>             | <u>cal.DoECAL1PortEx</u>                |
| Do ECAL 2-Port                                                                                                         | <u>SENS:CORR:COLL:CKIT 99</u>             | <u>cal.DoECAL2PortEx</u>                |
| Get ECAL Module Info                                                                                                   | <u>SENS:CORR:COLL:CKIT:INF?</u>           | <u>cal.GetECALModuleInfoEx</u>          |
| Test Module communication                                                                                              | None                                      | <u>cal.IsECALModuleFoundEx</u>          |

|                                                          |                                 |                                            |
|----------------------------------------------------------|---------------------------------|--------------------------------------------|
| Perform Module Orientation during calibration            | <u>SENS:CORR:PREF:ECAL:ORI</u>  | <u>cal.OrientECALModule</u>                |
| Maps ECAL Module to PNA Ports                            | <u>SENS:CORR:PREF:ECAL:PMAP</u> | <u>cal.ECALPortMapEx</u>                   |
| Confidence Check Parameter                               | <u>SENS:CORR:CCH:PAR</u>        | <u>cal.AcquireCalConfidenceCheckECALEX</u> |
| Confidence Check Acquire                                 | <u>SENS:CORR:CCHeck</u>         | <u>cal.AcquireCalConfidenceCheckECALEX</u> |
| Confidence Check Done                                    | <u>SENS:CORR:CCH:DONE</u>       | <u>cal.DoneCalConfidenceCheckECAL</u>      |
| Sets the internal state of the selected ECAL module.     | <u>CONT:ECAL:MOD:STATE</u>      |                                            |
| <b>Recall / Save / Apply a Calibration or Error Term</b> |                                 |                                            |
| Recall a Calibration                                     | <u>SENS:CORR:CSET</u>           | <u>app.Recall</u>                          |
| Apply a Calibration to a measurement                     | <u>SENS:CORR:CSET</u>           |                                            |
| Save a Calibration                                       | <u>SENS:CORR:CSET:SAVE</u>      | <u>app.Save</u>                            |
| Save or Recall an Error Term                             | <u>CALC:DATA Scorr</u>          | <u>Data Topic</u>                          |
| Read/ Write Cal Set data                                 | <u>SENS:CORR:CSET:DATA</u>      |                                            |
| Apply an Error Term after Uploading                      | <u>SENS:CORR:COLLect:APPLY</u>  |                                            |
| <b>Cal Sets</b>                                          |                                 |                                            |
| Create a Cal Set                                         | <u>SENS:CORR:CSET:CREate</u>    | <u>calMgr.CreateCalSet</u>                 |
| Delete a Cal Set                                         | <u>SENS:CORR:CSET:DEL</u>       | <u>calMgr.DeleteCalSet</u>                 |
| List Cal Sets                                            | <u>SENS:CORR:CSET:CAT?</u>      | <u>calMgr.GetCalSetCatalog</u>             |
| Get Cal Set Information                                  |                                 | <u>calMgr.GetCalSetUsageInfo</u>           |
| Select a Cal Set by GUID                                 | <u>SENS:CORR:CSET:GUID</u>      | <u>calMgr.GetCalSetByGUID</u>              |
| Select a Cal Set from a channel                          |                                 | <u>channel.SelectCalSet</u>                |
| Copy a Cal Set                                           |                                 | <u>CalSet.Copy</u>                         |
| Save a Cal Set                                           |                                 | <u>CalSet.Save</u>                         |
| Save Cal Sets                                            | <u>SENS:CORR:CSET:SAVE</u>      | <u>app.SaveCalSets</u>                     |
| Automatically save to User Cal Set                       | <u>SENS:CORR:PREF:CSET:SAVU</u> |                                            |
| Change the Description of a Cal Set                      | <u>SENS:CORR:CSET:DESC</u>      | <u>CalSet.Description</u>                  |
| Change the Name of a Cal Set                             | <u>SENS:CORR:CSET:NAME</u>      |                                            |
| Change the Contents of a Cal Set                         |                                 | <u>calset object</u>                       |
| Recall a Cal Set                                         |                                 | <u>app.Recall</u>                          |
| <b>Correction Settings</b>                               |                                 |                                            |
| Turn Correction ON OFF for a channel                     | <u>SENS:CORR</u>                | <u>chan.ErrorCorrection</u>                |

|                                                           |                                         |                                   |
|-----------------------------------------------------------|-----------------------------------------|-----------------------------------|
| Turn Correction ON OFF for a measurement                  | <u>CALC:CORR</u>                        | <u>meas.ErrorCORR</u>             |
| Catalog the correction types                              | <u>SENS:CORR:TYPE:CAT?</u>              | <u>calMgr.GetCalTypes</u>         |
| Set correction type (standard measurements)               | <u>CALC:CORR:TYPE</u>                   | <u>meas.CalibrationType</u>       |
| Set correction type (custom measurements)                 | <u>CALC:CORR:TYPE</u>                   | <u>meas.CalibrationTypeID</u>     |
| Interpolation ON OFF                                      | <u>SENS:CORR:INT</u>                    | <u>meas.InterpolateCorrection</u> |
| <b>Port Extensions</b>                                    |                                         |                                   |
| Extensions ON OFF                                         | <u>SENS:CORR:EXT</u>                    | <u>portExtension.State</u>        |
| Port 1 Extensions Value                                   | <u>SENS:CORR:EXT:PORT</u>               | <u>portExt.Port1</u>              |
| Port 2 Extensions Value                                   | <u>SENS:CORR:EXT:PORT</u>               | <u>portExt.Port2</u>              |
| Set Freq 1 2                                              | <u>SENS:CORR:EXT:PORT:FREQ</u>          | <u>Fix.PortFreq1</u>              |
| Set Loss 1 2                                              | <u>SENS:CORR:EXT:PORT:LOSS</u>          | <u>fix.PortLoss1</u>              |
| Use 1 2                                                   | <u>SENS:CORR:EXT:PORT:INCL</u>          | <u>fix.PortExtUse1</u>            |
| Set Loss at DC                                            | <u>SENS:CORR:EXT:PORT:LDC</u>           | <u>fix.PortLossDC</u>             |
| Relative Velocity                                         | <u>SENS:CORR:RVEL:COAX</u>              | <u>app.VelocityFactor</u>         |
| <b>Auto Port Extensions</b>                               |                                         |                                   |
| Measure OPEN or SHORT for Auto Port Ext.                  | <u>SENS:CORR:EXT:AUTO:MEASure</u>       | <u>AutoPortExtMeasure</u>         |
| Sets the frequencies used for Auto Port Ext. calculation. | <u>SENS:CORR:EXT:AUTO:CONFig</u>        | <u>AutoPortExtConfig</u>          |
| Include loss correction in Auto Port Ext.?                | <u>SENS:CORR:EXT:AUTO:LOSS</u>          | <u>AutoPortExtLoss</u>            |
| Include DC Offset in Auto Port Ext.?                      | <u>SENS:CORR:EXT:AUTO:DCOF</u>          | <u>AutoPortExtDCOffset</u>        |
| Enable specified port for Auto Port Ext..                 | <u>SENS:CORR:EXT:AUTO:PORT&lt;n&gt;</u> | <u>AutoPortExtState</u>           |
| Clears old port extension delay and loss data.            | <u>SENS:CORR:EXT:AUTO:RESet</u>         | <u>AutoPortExtReset</u>           |
| Set user span start frequency for Auto Port Ext.          | <u>SENS:CORR:EXT:AUTO:STARt</u>         | <u>AutoPortExtSearchStart</u>     |
| Set user span stop frequency for Auto Port Ext.           | <u>SENS:CORR:EXT:AUTO:STOP</u>          | <u>AutoPortExtSearchStop</u>      |
| <b>Fixturing Commands</b>                                 |                                         |                                   |
| Turn fixturing ON and OFF                                 | <u>CALC:FSIM:STAT</u>                   | <u>FixturingState</u>             |
| <b>2-Port Fixturing</b>                                   |                                         |                                   |
| Port matching ON and OFF                                  | <u>CALC:FSIM:SEND:PMC:STAT</u>          | <u>PortMatchingState</u>          |
| Sets Port Matching circuit model.                         | <u>CALC:FSIM:SEND:PMC:PORT:TYPE</u>     | <u>PortMatchingCktModel</u>       |



|                                               |                                                                                                       |                                  |
|-----------------------------------------------|-------------------------------------------------------------------------------------------------------|----------------------------------|
| Sets Port Matching 'S2P' file name.           | <u>CALC:FSIM:SEND:PMC:PORT:USER:FIL</u>                                                               | <u>strPortMatch_S2PFile</u>      |
| Sets Capacitance 'C' value.                   | <u>CALC:FSIM:SEND:PMC:PORT:PAR:C</u>                                                                  | <u>PortMatching_C</u>            |
| Sets Conductance 'G' value.                   | <u>CALC:FSIM:SEND:PMC:PORT:PAR:G</u>                                                                  | <u>PortMatching_G</u>            |
| Sets Inductance 'L' value.                    | <u>CALC:FSIM:SEND:PMC:PORT:PAR:L</u>                                                                  | <u>PortMatching_L</u>            |
| Sets Resistance 'R' value.                    | <u>CALC:FSIM:SEND:PMC:PORT:PAR:R</u>                                                                  | <u>PortMatching_R</u>            |
| De-embed ON and OFF                           | <u>CALC:FSIM:SEND:DEEM:PORT:STAT</u>                                                                  | <u>Port2PdeembedState</u>        |
| Sets De-embedding circuit model.              | <u>CALC:FSIM:SEND:DEEM:PORT</u>                                                                       | <u>Port2PdeembedCktModel</u>     |
| Sets De-embedding 'S2P' file name.            | <u>CALC:FSIM:SEND:DEEM:PORT:USER:FIL</u>                                                              | <u>strPort2Pdeembed_S2PFile</u>  |
| Port Impedance ON and OFF                     | <u>CALC:FSIM:SEND:ZCON:STAT</u>                                                                       | <u>PortArbzState</u>             |
| Port Z Real                                   | <u>CALC:FSIM:SEND:ZCON:PORT:REAL</u>                                                                  | <u>PortArbzReal</u>              |
| Port Z Imag                                   | <u>CALC:FSIM:SEND:ZCON:PORT:IMAG</u>                                                                  | <u>PortArbzImag</u>              |
| Port Z Real and Imag                          | <u>CALC:FSIM:SEND:ZCON:PORT:Z0</u>                                                                    | <u>PortArbzZ0</u>                |
| <b>4-Port Network Embed/De-embed commands</b> |                                                                                                       |                                  |
| Specifies the PNA / DUT topology              | <u>CALC:FSIM:EMB:TYPE</u>                                                                             | <u>Embed4PortTopology</u>        |
| Specifies the 4-port touchstone file          | <u>CALC:FSIM:EMB:NETW:FIL</u>                                                                         | <u>Embed4PortNetworkFilename</u> |
| Embed De-embed?                               | <u>CALC:FSIM:EMB:NETW:TYPE</u>                                                                        | <u>Embed4PortNetworkMode</u>     |
| Specify PNA port connections                  | <u>CALC:FSIM:EMB:TOP:A:PORT</u><br><u>CALC:FSIM:EMB:TOP:B:PORT</u><br><u>CALC:FSIM:EMB:TOP:C:PORT</u> | <u>Embed4PEmbed4PortList</u>     |
| Turn ON or OFF                                | <u>CALC:FSIM:EMB:STAT</u>                                                                             | <u>Embed4PortState</u>           |
| <b>Differential Port Arbitrary Impedance</b>  |                                                                                                       |                                  |
| Sets the impedance value                      | <u>CALC:FSIM:BAL:DZC:BPOR:Z0</u>                                                                      | <u>DiffZConvPortZ0</u>           |
| Sets real part of impedance                   | <u>CALC:FSIM:BAL:DZC:BPOR:REAL</u>                                                                    | <u>DiffZConvPortReal</u>         |
| Sets imaginary part of impedance              | <u>CALC:FSIM:BAL:DZC:BPOR:IMAG</u>                                                                    | <u>DiffZConvPortImag</u>         |
| Turn ON or OFF                                | <u>CALC:FSIM:BAL:DZC:STAT</u>                                                                         | <u>DiffZConvState</u>            |
| <b>Common Mode Port Arbitrary Impedance</b>   |                                                                                                       |                                  |
| Sets the impedance value                      | <u>CALC:FSIM:BAL:CZC:BPOR:Z0</u>                                                                      | <u>CmnModeZConvPortZ0</u>        |
| Sets real part of impedance                   | <u>CALC:FSIM:BAL:CZC:BPOR:REAL</u>                                                                    | <u>CmnModeZConvPortReal</u>      |
| Sets imaginary part of impedance              | <u>CALC:FSIM:BAL:CZC:BPOR:IMAG</u>                                                                    | <u>CmnModeZConvPortImag</u>      |
| Turn ON or OFF                                | <u>CALC:FSIM:BAL:CZC:STAT</u>                                                                         | <u>CmnModeZConvState</u>         |
| <b>Differential Port Matching</b>             |                                                                                                       |                                  |
| Sets type of circuit to embed.                | <u>CALC:FSIM:BAL:DMC:BPOR</u>                                                                         | <u>DiffPortMatchMode</u>         |

|                                      |                                             |                                              |
|--------------------------------------|---------------------------------------------|----------------------------------------------|
| Specifies the 2-port touchstone file | <u>CALC:FSIM:BAL:DMC:BPOR:USER:FIL</u>      | <u>DiffPortMatchUserFilename</u>             |
| Sets Capacitance value               | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:C</u>         | <u>DiffPortMatch_C</u>                       |
| Sets Conductance value               | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:G</u>         | <u>DiffPortMatch_G</u>                       |
| Sets Inductance value                | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:L</u>         | <u>DiffPortMatch_L</u>                       |
| Sets Resistance value                | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:R</u>         | <u>DiffPortMatch_R</u>                       |
| Turns ON/OFF                         | <u>CALC:FSIM:BAL:DMC:STAT</u>               | <u>DiffPortMatchState</u>                    |
| <b>Global Delta Match Cal</b>        |                                             |                                              |
| Initiate Cal                         | <u>SENS:CORR:COLL:GUID:DMAT</u>             | <u>guid.GenerateGlobalDeltaMatchSequence</u> |
| Read ports that require Cal          | <u>SENS:CORR:COLL:GUID:DMAT:APPLY:PORT?</u> | <u>guid.PortsNeedingDeltaMatch</u>           |
| Apply a Cal                          | <u>SENS:CORR:COLL:GUID:DMAT:APPLY</u>       | <u>guid.ApplyDeltaMatchFromCalSet</u>        |
| <b>Manage and Modify Cal Kits</b>    |                                             |                                              |
| Set a Cal Kit Active                 | <u>SENS:CORR:COLL:CKIT</u>                  | <u>app.CalKitType</u>                        |
| Clear all Cal Kits from PNA          | <u>SENS:CORR:CKIT:CLE</u>                   |                                              |
| Get a Handle to the Active Cal Kit   |                                             | <u>app.ActiveCalKit</u>                      |
| Save All Cal Kits after Modifying    |                                             | <u>app.SaveKits</u>                          |
| Load collection of Kits              | <u>SENS:CORR:CKIT:LOAD</u>                  |                                              |
| Load (Recall) All Cal Kits           |                                             | <u>app.RecallKits</u>                        |
| Import a specified kit.              | <u>SENS:CORR:CKIT:IMP</u>                   |                                              |
| Restore Cal Kit Default              | <u>SENS:CORR:COLL:CKIT:RESet</u>            |                                              |
| Restore ALL Cal Kits Default         | <u>SENS:CORR:CKIT:INITialize</u>            |                                              |
| Build a Hybrid Cal Kit               |                                             | <u>app.BuildHybridKit</u>                    |
| Set the Name of a Cal Kit            | <u>SENS:CORR:COLL:CKIT:NAME</u>             | <u>calKit.Name</u>                           |
| Set a description of a Cal Kit       | <u>SENS:CORR:COLL:CKIT:DESC</u>             |                                              |
| Get the amount of installed kits     | <u>SENS:CORR:CKIT:COUNt?</u>                |                                              |
| Set the Port Label of a Cal Kit      |                                             | <u>calKit.Portlabel</u>                      |
| <b>Modify Cal Standards</b>          |                                             |                                              |
| Select a Cal Standard                | <u>SENS:CORR:COLL:CKIT:STAN</u>             | <u>calkit.GetCalStandard</u>                 |
| Delete a standard                    | <u>SENS:CORR:COLL:CKIT:STAN:REM</u>         |                                              |
| Change description of a standard     | <u>SENS:CORR:COLL:CKIT:STAN:SDES</u>        |                                              |
| Assign a Class to a Standard         | <u>SENS:CORR:COLL:CKIT:ORD1</u>             | <u>calKit.StandardForClass</u>               |
| Set Standard Type                    | <u>SENS:CORR:COLL:CKIT:STAN:TYPE</u>        | <u>calstd.Type</u>                           |
| Add connector family name            | <u>SENS:CORR:COLL:CKIT:CONN:ADD</u>         |                                              |
| Delete connector family name         | <u>SENS:CORR:COLL:CKIT:CONN:DEL</u>         |                                              |

|                                                                                               |                                        |                                     |
|-----------------------------------------------------------------------------------------------|----------------------------------------|-------------------------------------|
| List connector family names used in a Cal Kit                                                 | <u>SENS:CORR:COLL:CKIT:CONN:CAT?</u>   |                                     |
| Replace connector family name.                                                                | <u>SENS:CORR:COLL:CKIT:CONN:FNAM</u>   |                                     |
| Assign connector family name to a standard                                                    | <u>SENS:CORR:COLL:CKIT:CONN:SNAME</u>  |                                     |
| Set Delay                                                                                     | <u>SENS:CORR:COLL:CKIT:STAN:DEL</u>    | <u>calstd.Delay</u>                 |
| Set Loss                                                                                      | <u>SENS:CORR:COLL:CKIT:STAN:LOSS</u>   | <u>calstd.loss</u>                  |
| Set Impedance                                                                                 | <u>SENS:CORR:COLL:CKIT:STAN:IMP</u>    | <u>calstd.Z0</u>                    |
| Set Max Frequency                                                                             | <u>SENS:CORR:COLL:CKIT:STAN:FMAX</u>   | <u>calstd.MaximumFrequency</u>      |
| Set Min Frequency                                                                             | <u>SENS:CORR:COLL:CKIT:STAN:FMIN</u>   | <u>calstd.MinimumFrequency</u>      |
| Set Label                                                                                     | <u>SENS:CORR:COLL:CKIT:STAN:LAB</u>    | <u>calstd.Label</u>                 |
| Set Medium (coax   waveguide)                                                                 | <u>SENS:CORR:COLL:CKIT:STAN:CHAR</u>   | <u>calstd.Medium</u>                |
| Set Capacitance (C0 to C3)                                                                    | <u>SENS:CORR:COLL:CKIT:STAN:C0</u>     | <u>calstd.C0</u>                    |
| Set Inductance (L0 to L3)                                                                     | <u>SENS:CORR:COLL:CKIT:STAN:L0</u>     | <u>calstd.L0</u>                    |
| Set Arbitrary Impedance (TZReal, TZImag)                                                      | <u>SENS:CORR:COLL:CKIT:STAN:TZReal</u> | <u>calstd.TZReal</u>                |
| <b>Source Power Calibration</b>                                                               |                                        |                                     |
| GPIB Power Meter Address                                                                      | <u>SYST:COMM:GPIB:PMET:ADDR</u>        | <u>pwrCal.PowerMeterGPIBAddress</u> |
| Set source power cal method                                                                   | <u>SOUR:POW:CORR:COLL:METH</u>         | <u>SetCallInfo2 Method</u>          |
| Turn correction ON OFF                                                                        | <u>SOUR:POW:CORR</u>                   | <u>SourcePowerCorrection</u>        |
| Applies correction values after completing a source power cal acquisition sweep.              | <u>SOUR:POW:CORR:COLL:SAVE</u>         | <u>ApplyPowerCorrectionValues</u>   |
| Returns the currently selected power sensor channel (A or B) for use at a specific frequency. |                                        | <u>PowerAcquisitionDevice</u>       |
| Set power level                                                                               | <u>SOUR:POW:CORR:LEV</u>               | <u>CalPower</u>                     |
| Set power offset                                                                              | <u>SOUR:POW:CORR:OFFS</u>              | <u>SourcePowerCalPowerOffset</u>    |
| Set settling tolerance                                                                        | <u>SOUR:POW:CORR:COLL:AVER:NTOL</u>    | <u>ReadingsTolerance</u>            |
| Set max readings for settling                                                                 | <u>SOUR:POW:CORR:COLL:AVER:COUNT</u>   | <u>ReadingsPerPoint</u>             |
| Set accuracy tolerance                                                                        | <u>SOUR:POW:CORR:COLL:ITER:NTOL</u>    | <u>IterationsTolerance</u>          |
| Set max readings for accuracy                                                                 | <u>SOUR:POW:CORR:COLL:ITER:COUNT</u>   | <u>MaximumIterationsPerPoint</u>    |
| Turn ON OFF display of readings                                                               | <u>SOUR:POW:CORR:COLL:DISP</u>         | <u>SetCallInfo2 Method</u>          |
| Initiates a source power cal acquisition.                                                     | <u>SOUR:POW:CORR:COLL:ACQ</u>          | <u>AcquirePowerReadings</u>         |


|                                                                            |                                            |                                       |
|----------------------------------------------------------------------------|--------------------------------------------|---------------------------------------|
| Aborts a source power cal acquisition sweep that is currently in progress. | <u>SOUR:POW:CORR:COLL:ABOR</u>             | <u>AbortPowerAcquisition</u>          |
| Launches the Power Meter Settings dialog on the PNA.                       |                                            | <u>LaunchPowerMeterSettingsDialog</u> |
| Frequency checking (ON OFF)                                                | <u>SOUR:POW:CORR:COLL:FCH</u>              | <u>UsePowerSensorFrequencyLimits</u>  |
| Check test port power                                                      |                                            | <u>CheckPower</u>                     |
| <b>Power Sensor</b>                                                        |                                            |                                       |
| Minimum Frequency                                                          | <u>SOUR:POW:CORR:COLL:&lt;&gt;SEN</u>      | <u>MinimumFrequency</u>               |
| Maximum Frequency                                                          | <u>SOUR:POW:CORR:COLL:&lt;&gt;SEN</u>      | <u>MaximiumFrequency</u>              |
| Power meter channel                                                        |                                            | <u>PowerMeterChannel</u>              |
| Set sensor cal factor                                                      | <u>SOUR:POW:CORR:COLL:&lt;&gt;SEN:RCF</u>  | <u>ReferenceCalFactor</u>             |
| Set table type                                                             | <u>SOUR:POW:CORR:COLL:TABL &lt;&gt;SEN</u> |                                       |
| Read/Write cal data                                                        | <u>SOUR:POW:CORR:DATA</u>                  | <u>See Data</u>                       |
| Use Loss table?                                                            | <u>SOUR:POW:CORR:COLL:TABL:LOSS</u>        | <u>UsePowerLossSegments</u>           |
| <b>Cal Factor Table</b>                                                    | <u>SOUR:POW:CORR:COLL:TABL:SEL</u>         | <u>CalFactorSegments Collection</u>   |
| Read number of segments in table                                           | <u>SOUR:POW:CORR:COLL:TABL:POIN?</u>       | <u>Count</u>                          |
| Segment number                                                             |                                            | <u>SegmentNumber</u>                  |
| Add segment                                                                |                                            | <u>Add</u>                            |
| Cal factor of the segment                                                  | <u>SOUR:POW:CORR:COLL:TABL:DATA</u>        | <u>CalFactor</u>                      |
| Frequency of the segment                                                   | <u>SOUR:POW:CORR:COLL:TABL:FREQ</u>        | <u>Frequency</u>                      |
| <b>Power Loss Table</b>                                                    | <u>SOUR:POW:CORR:COLL:TABL:SEL</u>         | <u>PowerLossSegments Collection</u>   |
| Read number of segments in table                                           | <u>SOUR:POW:CORR:COLL:TABL:POIN?</u>       | <u>Count</u>                          |
| Segment number                                                             |                                            | <u>SegmentNumber</u>                  |
| Add segment                                                                |                                            | <u>Add</u>                            |
| Frequency                                                                  | <u>SOUR:POW:CORR:COLL:TABL:FREQ</u>        | <u>Frequency</u>                      |
| Loss value                                                                 | <u>SOUR:POW:CORR:COLL:TABL:DATA</u>        | <u>Loss</u>                           |
| <b>Receiver Cal</b>                                                        |                                            |                                       |
| Set offset from test port power                                            | <u>SENS:CORR:RPOWER:OFFSet[:AMPLitude]</u> | <u>LogMagnitudeOffset</u>             |
| Set cal method to receiver cal                                             | <u>SENS:CORR:COLL:METH RPOWER</u>          | <u>DoReceiverPowerCal</u>             |
| Take measurement                                                           | <u>SENS:CORR:COLL[:ACQ] POWER</u>          | N/A                                   |
| Turn receiver cal ON   OFF                                                 | <u>SENS:CORR[:STATe] ON OFF</u>            | <u>Error Correction</u>               |

---

|                                          |                                     |                              |
|------------------------------------------|-------------------------------------|------------------------------|
| Do interpolation                         | <u>SENS:CORR:INT[:STATe] ON OFF</u> | <u>InterpolateCorrection</u> |
| <b>Retrieve and Put Calibration Data</b> |                                     |                              |
| Retrieve Cal Data from the PNA           | <u>CALC:DATA scorr?</u> or SDIV?    | <u>see Data Topic</u>        |
| Put Cal Data in the PNA                  | <u>CALC:DATA scorr</u> or SDIV      | <u>see Data Topic</u>        |

| File        | View | Chan | Sweep | Cal  | Trace | Scale | Marker | System             | Mixer | Data |
|-------------|------|------|-------|------|-------|-------|--------|--------------------|-------|------|
| Description |      |      |       | SCPI |       |       |        | COM (remove frame) |       |      |

**Power | Average | Offset | Manage | IF Access | Interface Control | E5091A**

|                                                                                                    |                                |                                       |
|----------------------------------------------------------------------------------------------------|--------------------------------|---------------------------------------|
| Channel Preset                                                                                     | none - (See <u>SYST:PRES</u> ) | <u>app.Preset</u>                     |
| Start Freq                                                                                         | <u>SENS:FREQ:STAR</u>          | <u>chan.StartFrequency</u>            |
| Stop Freq                                                                                          | <u>SENS:FREQ:STOP</u>          | <u>chan.StopFrequency</u>             |
| Center Freq                                                                                        | <u>SENS:FREQ:CENT</u>          | <u>chan.CenterFrequency</u>           |
| Span                                                                                               | <u>SENS:FREQ:SPAN</u>          | <u>chan.FrequencySpan</u>             |
| CW Frequency                                                                                       | <u>SENS:FREQ:CW</u>            | <u>chan.CWFrequency</u>               |
| <b>Power Settings</b>                                                                              |                                |                                       |
| Power ON   OFF                                                                                     | <u>OUTP</u>                    | <u>app.SourcePowerState</u>           |
| Power Value                                                                                        | <u>SOUR:POW1</u>               | <u>chan.TestPortPower</u>             |
| Port Selection                                                                                     | <u>SENS:SWE:SRCP</u>           | <u>chan.TestPortPower</u>             |
| Couple Ports OFF   ON                                                                              | <u>SOUR:POW:COUP</u>           | <u>chan.CouplePorts</u>               |
| Attenuator Mode Auto Manual                                                                        | <u>SOUR:POW:ATT:Auto</u>       | <u>chan.Attenuator</u>                |
| Attenuation Value                                                                                  | <u>SOUR:POW:ATT</u>            | <u>chan.AttenuatorMode</u>            |
| Power Slope ON   OFF                                                                               | <u>SOUR:POW:SLOP:STAT</u>      | <u>app.PowerSlope</u>                 |
| Power Slope Value                                                                                  | <u>SOUR:POW:SLOP</u>           | <u>app.PowerSlope</u>                 |
| Receiver Attenuation                                                                               | <u>SENS:POW:ATT</u>            | <u>chan.ReceiverAttenuator</u>        |
| <b>Averaging</b>                                                                                   |                                |                                       |
| Average ON OFF                                                                                     | <u>SENS:AVER</u>               | <u>chan.Average</u>                   |
| Average Factor                                                                                     | <u>SENS:AVER:COUN</u>          | <u>chan.AveragingFactor</u>           |
| Return the Average Count                                                                           |                                | <u>chan.AveragingCount</u>            |
| Average Restart                                                                                    | <u>SENS:AVER:CLE</u>           | <u>chan.AveragingRestart</u>          |
| <b>Frequency Offset</b>                                                                            |                                |                                       |
| Offset mode ON   OFF                                                                               | <u>SENS:OFFS:STAT</u>          | <u>chan.FrequencyOffsetState</u>      |
|  fset Frequency | <u>SENS:OFFS:OFFS</u>          | <u>chan.FrequencyOffsetFrequency</u>  |
| Read Offset Start Frequency                                                                        | <u>SENS:OFFS:STAR?</u>         |                                       |
| Read Offset Stop Frequency                                                                         | <u>SENS:OFFS:STOP?</u>         |                                       |
| Set Offset Multiplier                                                                              | <u>SENS:OFFS:MULT</u>          | <u>chan.FrequencyOffsetMultiplier</u> |
| Set Offset Divisor                                                                                 | <u>SENS:OFFS:DIV</u>           | <u>chan.FrequencyOffsetDivisor</u>    |
| Set CW Override                                                                                    | <u>SENS:OFFS:CW</u>            | <u>chan.FrequencyOffsetCWOverride</u> |
| Test Set Switch                                                                                    | <u>ROUT:PATH:LOOP:R1</u>       | <u>chan.R1InputPath</u>               |
| <b>Manage Channels</b>                                                                             |                                |                                       |
| Add                                                                                                |                                | <u>chans.Add</u>                      |
| Make Active                                                                                        |                                | <u>app.ActiveChannel</u>              |
| Read Channel Number                                                                                |                                | <u>chan.ChannelNumber</u>             |
| Read UNUSED channel numbers                                                                        |                                | <u>chans.UnusedChannelNumbers</u>     |

|                                                |                                                    |                                                 |
|------------------------------------------------|----------------------------------------------------|-------------------------------------------------|
| Read used channel numbers                      |                                                    | <a href="#"><u>chans.UsedChannelNumbers</u></a> |
| Read Number of Channels                        |                                                    | <a href="#"><u>chans.Count</u></a>              |
| Copy a Channel                                 |                                                    | <a href="#"><u>chan.CopyToChannel</u></a>       |
| <b>IF Access</b>                               |                                                    |                                                 |
| Set gain state (Auto   Manual)                 | <a href="#"><u>SENS:IF:GAIN:ALL</u></a>            | <a href="#"><u>chan.IFGainMode</u></a>          |
| Set gain level                                 | <a href="#"><u>SENS:IF:GAIN:LEVel</u></a>          | <a href="#"><u>chan.IFGainLevel</u></a>         |
| Read gain level                                | <a href="#"><u>SENS:IF:GAIN?</u></a>               | <a href="#"><u>chan.IFGainLevel</u></a>         |
| Filter taps count                              | <a href="#"><u>SENS:IF:FILT:SAMP:COUN</u></a>      | <a href="#"><u>IFFilterSampleCount</u></a>      |
| Filter tap mode (Auto/Manual)                  | <a href="#"><u>SENS:IF:FILT:SAMP:COUN:MODE</u></a> | <a href="#"><u>IFFilterSource</u></a>           |
| IF filter sample period                        | <a href="#"><u>SENS:IF:FILT:SAMP:PERiod</u></a>    | <a href="#"><u>IFFilterSamplePeriod</u></a>     |
| List valid sample periods                      | <a href="#"><u>SENS:IF:FILT:SAMP:PER:CAT</u></a>   | <a href="#"><u>IFFilterSamplePeriodList</u></a> |
| Sample period mode (Auto/Manual)               | <a href="#"><u>SENS:IF:FILT:SAMP:PER:MOD</u></a>   | <a href="#"><u>IFFilterSamplePeriodMode</u></a> |
| IF gate state (ON / OFF)                       | <a href="#"><u>SENS:IF:GATE:STATe</u></a>          | <a href="#"><u>IFGateEnable</u></a>             |
| Set IF source path                             | <a href="#"><u>SENS:IF:SOUR:PATH</u></a>           | <a href="#"><u>chan.IFSourcePath</u></a>        |
| <b>Interface Control</b>                       |                                                    |                                                 |
| Interface Control ON OFF                       | <a href="#"><u>Control:Interface:State</u></a>     | <a href="#"><u>IC.State</u></a>                 |
| Recall Interface Control file                  | <a href="#"><u>Control:Interface:Config</u></a>    | <a href="#"><u>IC.ConfigurationFile</u></a>     |
| <b>E5091A Test Set Control</b>                 |                                                    |                                                 |
| Reads the number of ports                      | <a href="#"><u>SENS:MULT:COUN?</u></a>             | <a href="#"><u>e5091.NumberOfPorts</u></a>      |
| Turns ON and OFF the property display          | <a href="#"><u>SENS:MULT1:DISP</u></a>             | <a href="#"><u>e5091.ShowProperties</u></a>     |
| Sets the control lines of the specified E5091A | <a href="#"><u>SENS:MULT1:TSET:OUTP</u></a>        | <a href="#"><u>e5091.Controllines</u></a>       |
| Switches Port 1                                | <a href="#"><u>SENS:MULT:TSET9:PORT1</u></a>       | <a href="#"><u>e5091.OutputPort</u></a>         |
| Switches Port 2                                | <a href="#"><u>SENS:MULT:TSET9:PORT2</u></a>       | <a href="#"><u>e5091.OutputPort</u></a>         |
| Switches Port 3                                | <a href="#"><u>SENS:MULT:TSET9:PORT3</u></a>       | <a href="#"><u>e5091.OutputPort</u></a>         |
| Switches Port 4                                | <a href="#"><u>SENS:MULT:TSET9:PORT4</u></a>       | <a href="#"><u>e5091.OutputPort</u></a>         |
| Turns ON/OFF switching.                        | <a href="#"><u>SENS:MULT:STATe</u></a>             | <a href="#"><u>e5091.Enabled</u></a>            |
| Return ID of the tetset                        |                                                    | <a href="#"><u>ID Property</u></a>              |



## Code Translator Application

---

The Code Translator (CXL) Application allows you to control the PNA using your 8753, 872x, or 8510 (Legacy) GPIB test programs. The CXL Application runs on the PNA and processes each legacy command, real time, by first recognizing it as a valid legacy commands, and then executing the equivalent PNA command if one exists. The CXL Application will also help translate your Legacy programs into PNA SCPI and COM commands.

The CXL Application works with HP-VEE, Visual Basic, and RMB programs. The CXL Application must be used with PNA revision firmware A.04.00 or later.

---


**Note:** CXL does NOT translate all legacy commands. It is currently available "AS-IS" to HELP with your Legacy-to-PNA code translation. Please provide feedback on your use of the application.


---

### Installing the CXL Application

Download the CXL application from <http://na.tm.agilent.com/pna/cxl.html>. To install the CXL application, double click on the InstallShield package icon.


The CXL application has its own help file that includes a command cross-reference for 8510/8753/872x models to PNA commands.

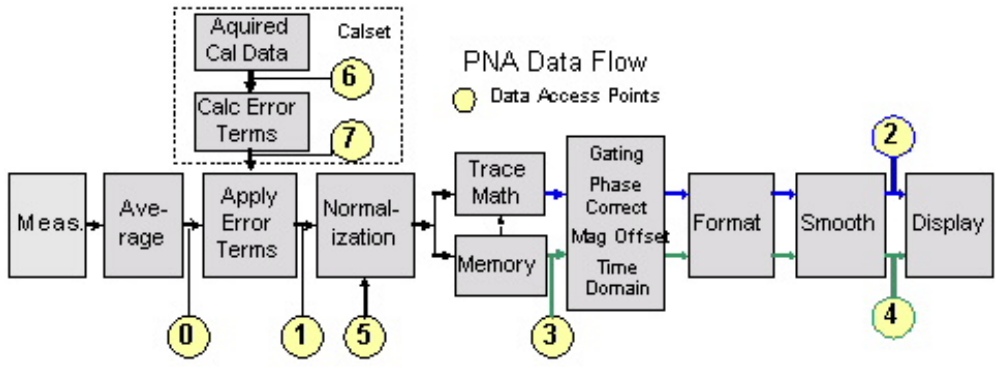

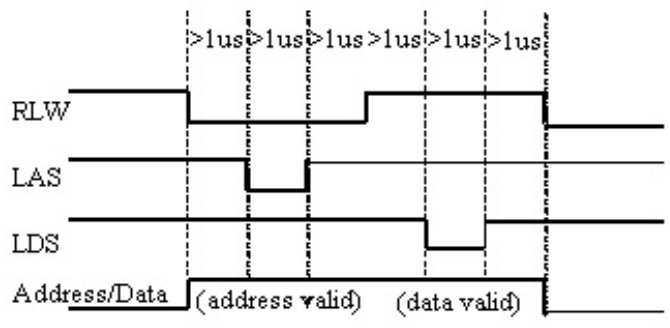



**Measurement | Cal | Power Cal | Custom**

See a [map](#) of the data access locations

|                                                                                                                                                  |                                     |                                              |
|--------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|----------------------------------------------|
| Get X-Axis values (variant)                                                                                                                      | <a href="#">SENS:X:VAL</a>          | <a href="#">Get X-axis Values</a>            |
| Get X-Axis values (typed)                                                                                                                        |                                     | <a href="#">Get X-Axis Values 2</a>          |
| Get X-Axis values (Meas object)                                                                                                                  |                                     | <a href="#">Get XAxisValues</a>              |
| <b>Get Measurement Data FROM the Analyzer</b>                                                                                                    |                                     |                                              |
| Get <b>complex</b> data from the specified location.                                                                                             |                                     | <a href="#">IArrayTrans.getComplex</a>       |
| Get typed <b>NAComplex</b> data from the specified location.                                                                                     |                                     | <a href="#">IArrayTrans.getNAComplex</a>     |
| Get <b>data pairs</b> from the specified location.                                                                                               |                                     | <a href="#">IArrayTrans.getPairedData</a>    |
| Get <b>scalar</b> data from the specified location.                                                                                              |                                     | <a href="#">IArrayTrans.getScalar</a>        |
| Get <b>variant</b> data from the specified location in a SPECIFIED FORMAT.                                                                       |                                     | <a href="#">meas.GetData</a>                 |
| Specifies ASCII or REAL type for data transfers                                                                                                  | <a href="#">Format:Data</a>         |                                              |
| Get complex or formatted data from the measurement or memory result buffer                                                                       | <a href="#">Calc:Data</a>           |                                              |
| Get SnP data                                                                                                                                     | <a href="#">Calc:Data:SnP</a>       | <a href="#">meas.GetSnPData</a>              |
| <b>Put Measurement Data INTO the Analyzer</b>                                                                                                    |                                     |                                              |
| Put <b>complex</b> data into the specified location.                                                                                             |                                     | <a href="#">IArrayTrans.putComplex</a>       |
| Put typed <b>NAComplex</b> data into the specified location.                                                                                     |                                     | <a href="#">IArrayTrans.putNAComplex</a>     |
| Put <b>scalar</b> data into the measurement result location.                                                                                     |                                     | <a href="#">IArrayTrans.putScalar</a>        |
|  Put <b>complex Variant</b> data into the specified location. |                                     | <a href="#">IArrayTrans.putDataComplex</a>   |
| Put complex or formatted data into the measurement or memory result buffer                                                                       | <a href="#">Calc:Data</a>           |                                              |
| <b>Get Calibration Data FROM the Analyzer</b>                                                                                                    |                                     |                                              |
| Get <b>complex Error Term</b> data                                                                                                               |                                     | <a href="#">Get ErrorTermComplexByString</a> |
| Get <b>variant Error Term</b> data                                                                                                               | <a href="#">SENS:CORR:CSET:DATA</a> | <a href="#">GetErrorTermByString</a>         |
| Get <b>complex Standard</b> data                                                                                                                 |                                     | <a href="#">GetStandardComplexByString</a>   |
| Get <b>variant Standard</b> data                                                                                                                 |                                     | <a href="#">GetStandardByString</a>          |
| <b>Put Calibration Data INTO the Analyzer</b>                                                                                                    |                                     |                                              |
| Put <b>complex Error Term</b> data                                                                                                               |                                     | <a href="#">PutErrorTermComplexByString</a>  |

|                                            |                            |                                       |
|--------------------------------------------|----------------------------|---------------------------------------|
| Put <b>variant Error Term</b> data         | <u>SENS:CORR:CSET:DATA</u> | <u>PutErrorTermByString</u>           |
| Put <b>complex Standard</b> data           |                            | <u>PutStandardComplexByString</u>     |
| Put <b>variant Standard</b> data           |                            | <u>PutStandardByString</u>            |
| <b>Power Calibration Data</b>              |                            |                                       |
| Get variant cal data                       | <u>SOUR:POW:CORR:DATA</u>  | <u>Get SourcePowerCalDataEx</u>       |
| Get typed cal data                         | <u>SOUR:POW:CORR:DATA</u>  | <u>Get SourcePowerCalDataScalarEx</u> |
| Put variant cal data                       | <u>SOUR:POW:CORR:DATA</u>  | <u>Put SourcePowerCalDataEx</u>       |
| Put typed cal data                         | <u>SOUR:POW:CORR:DATA</u>  | <u>Put SourcePowerCalDataScalarEx</u> |
| <b>Get and Put Custom Measurement Data</b> |                            |                                       |
| Get and Put Custom data                    | <u>Calc:Data</u>           | <u>IArrayTransfer2 Interface</u>      |

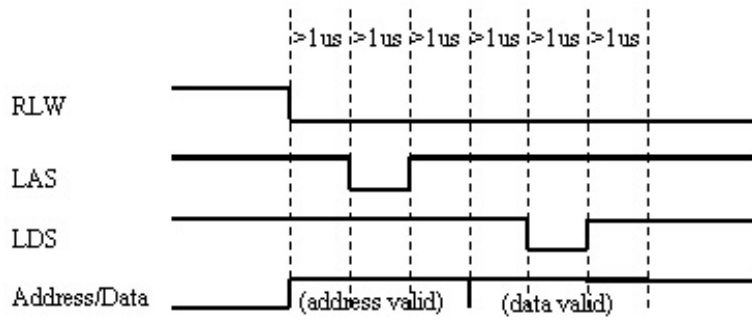

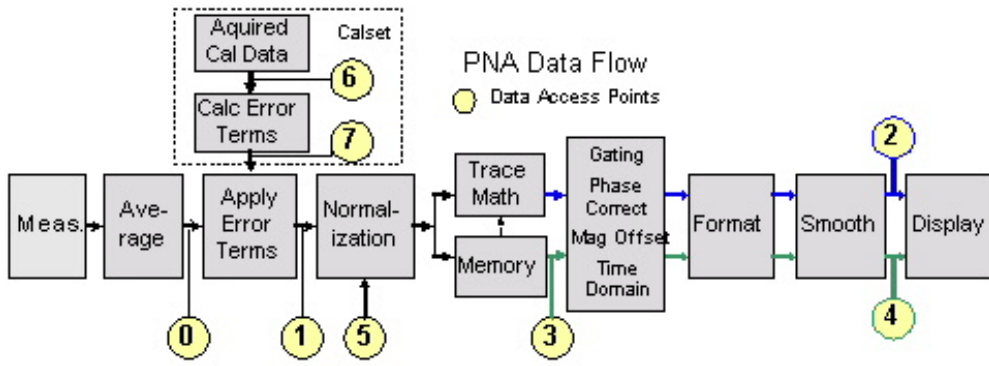


|                                                          |                                |                                  |
|----------------------------------------------------------|--------------------------------|----------------------------------|
| Save Instrument States (.cst, .sta, .cal) and .SnP files | <u>MMEemory:STORe</u>          | <u>app.Save</u>                  |
| Read SnP data                                            | <u>CALC:DATA:SnP</u>           | <u>meas.Get SnPData</u>          |
| Recall Files                                             | <u>MMEemory:LOAD</u>           | <u>app.recall</u>                |
| Sets format for .SnP files                               | <u>MMEM:STOR:TRAC:FORM:SNP</u> | <u>pref.SnPFormat</u>            |
| Saves formatted trace data to .cti file                  | <u>MMEM:STOR:CITI:FORM</u>     | <u>app.SaveCitiFormattedData</u> |
| Saves unformatted trace data to .cti file                | <u>MMEM:STOR:CITI:DATA</u>     | <u>app.SaveCitiDataData</u>      |
| Sets format for .cti files                               | <u>MMEM:STOR:TRAC:FORM:CIT</u> | <u>pref.CitiContents</u>         |
| Sets content for .cti files                              | <u>MMEM:STOR:TRAC:CONT:CIT</u> | <u>pref.CitiFormat</u>           |
| <b>Manage Files</b>                                      |                                |                                  |
| List Files                                               | <u>MMEemory:CATalog</u>        |                                  |
| Copy Files                                               | <u>MMEemory:COPY</u>           |                                  |
| Move Files                                               | <u>MMEemory:MOVE</u>           |                                  |
| Delete Files                                             | <u>MMEemory:DELeTe</u>         |                                  |
| <b>Manage Folders</b>                                    |                                |                                  |
| Change                                                   | <u>MMEemory:CDIRectory</u>     |                                  |
| Delete                                                   | <u>MMEemory:RDIRectory</u>     |                                  |
| Make                                                     | <u>MMEemory:MDIRectory</u>     |                                  |
| <b>Print</b>                                             |                                |                                  |
| Print                                                    | <u>HCOPY</u>                   | <u>app.DoPrint</u>               |
| Print to File                                            | <u>HCOPY:FILE</u>              | <u>app.PrintToFile</u>           |



**Function | Search**

|                                                                                                         |                                               |                                           |
|---------------------------------------------------------------------------------------------------------|-----------------------------------------------|-------------------------------------------|
| ON OFF                                                                                                  | <a href="#">CALC:MARK</a>                     | <a href="#">meas.MarkerState</a>          |
| Delete All Markers                                                                                      | <a href="#">CALC:MARK:AOFF</a>                | <a href="#">meas.DeleteAllMarkers</a>     |
| Delete Marker                                                                                           |                                               | <a href="#">meas.DeleteMarker</a>         |
| Viewing Marker readouts                                                                                 | <a href="#">View Topic</a>                    | <a href="#">View Topic</a>                |
| Interpolate All Markers                                                                                 |                                               | <a href="#">meas.Interpolate</a>          |
| Interpolate Individ. Marker                                                                             | <a href="#">CALC:MARK:DISC</a>                | <a href="#">mark.Interpolated</a>         |
| Type (Normal   Fixed)                                                                                   | <a href="#">CALC:MARK:TYPE</a>                | <a href="#">mark.Type</a>                 |
| Format All Markers                                                                                      |                                               | <a href="#">meas.MarkerFormat</a>         |
| Format Individ. Marker                                                                                  | <a href="#">CALC:MARK:FORM</a>                | <a href="#">mark.Format</a>               |
| Get a handle to Ref marker                                                                              |                                               | <a href="#">meas.GetReferenceMarker</a>   |
| Reference Marker On   Off                                                                               | <a href="#">CALC:MARK:REF</a>                 | <a href="#">meas.ReferenceMarkerState</a> |
| Coupled Markers                                                                                         | <a href="#">CALC:MARK:COUP</a>                | <a href="#">app.CoupledMarkers</a>        |
| Delta Marker                                                                                            | <a href="#">CALC:MARK:DELT</a>                | <a href="#">mark.DeltaMarker</a>          |
| Read/Set Data Point number                                                                              |                                               | <a href="#">mark.BucketNumber</a>         |
| Read/Set X-axis value                                                                                   | <a href="#">CALC:MARK:X</a>                   | <a href="#">mark.Stimulus</a>             |
| Read/Set Y-axis value                                                                                   | <a href="#">CALC:MARK:Y</a>                   | <a href="#">mark.Value</a>                |
| <b>Function</b>                                                                                         |                                               |                                           |
| Marker=> Center, Span, and so forth                                                                     | <a href="#">CALC:MARK:SET</a>                 |                                           |
| Marker=> Center (Freq)                                                                                  |                                               | <a href="#">mark.SetCenter</a>            |
| Marker=> CW Freq                                                                                        |                                               | <a href="#">mark.SetCW</a>                |
| Marker=> Start (Freq)                                                                                   |                                               | <a href="#">mark.SetStart</a>             |
| Marker=> Stop (Freq)                                                                                    |                                               | <a href="#">mark.SetStop</a>              |
| Marker=> Elect. Delay                                                                                   |                                               | <a href="#">mark.SetElectricalDelay</a>   |
|  Marker=> Ref. Level |                                               | <a href="#">mark.SetReferenceLevel</a>    |
| <b>Search</b>                                                                                           |                                               |                                           |
| Execute Search                                                                                          | <a href="#">CALC:MARK:FUNC:EXEC</a>           |                                           |
| Select Search Function                                                                                  | <a href="#">CALC:MARK:FUNC</a>                |                                           |
| Maximum                                                                                                 | <a href="#">CALC:MARK:FUNC</a>                | <a href="#">mark.SearchMax</a>            |
| Minimum                                                                                                 | <a href="#">CALC:MARK:FUNC</a>                | <a href="#">mark.SearchMin</a>            |
| Target (Value)                                                                                          | <a href="#">CALC:MARK:TARG</a>                | <a href="#">mark.TargetValue</a>          |
| Excursion Value                                                                                         | <a href="#">CALC:MARK:FUNC:APE:EXC</a>        | <a href="#">mark.PeakExcursion</a>        |
| Threshold Value                                                                                         | <a href="#">CALC:MARK:FUNC:APE:THR</a>        | <a href="#">mark.PeakThreshold</a>        |
| Assign Marker to Domain                                                                                 | <a href="#">CALC:MARK:FUNC:DOM:USER</a>       | <a href="#">mark.UserRange</a>            |
| Domain Range Start                                                                                      | <a href="#">CALC:MARK:FUNC:DOM:USER:START</a> | <a href="#">mark.UserRangeMin</a>         |
| Domain Range Stop                                                                                       | <a href="#">CALC:MARK:FUNC:DOM:USER:STOP</a>  | <a href="#">mark.UserRangeMax</a>         |

|                         |                            |                                   |
|-------------------------|----------------------------|-----------------------------------|
| Tracking                | <u>CALC:MARK:FUNC:TRAC</u> | <u>mark.Tracking</u>              |
| Bandwidth (Target)      | <u>CALC:MARK:TARG</u>      | <u>meas.BandwidthTarget</u>       |
| Search Filter Bandwidth | <u>CALC:MARK:BWID</u>      | <u>meas.SearchFilterBandwidth</u> |
| Read Filter BandWidth   | <u>CALC:MARK:BWID</u>      | <u>meas.FilterBW</u>              |
| Read Filter Center Freq | <u>CALC:MARK:BWID</u>      | <u>meas.FilterCF</u>              |
| Read Filter Loss        | <u>CALC:MARK:BWID</u>      | <u>meas.FilterLoss</u>            |
| Read Filter Q           | <u>CALC:MARK:BWID</u>      | <u>meas.FilterQ</u>               |

**Create | Configure | SMC | VMC**For Frequency Offset ([opt.080](#)) commands see [Chan / Offset](#)**Create or Load a Mixer Measurement (See [SCPI](#) and [COM](#) examples)**

|                             |                               |                                               |
|-----------------------------|-------------------------------|-----------------------------------------------|
| Create a custom measurement | <a href="#">CALC:CUST:DEF</a> | <a href="#">App.CreateCustomMeasurementEx</a> |
| Change a custom measurement | <a href="#">CALC:CUST:MOD</a> |                                               |
| Load a .mxr file            | <a href="#">SENS:MIX:LOAD</a> | <a href="#">LoadFile</a>                      |
| Save a .mxr file            | <a href="#">SENS:MIX:SAVE</a> | <a href="#">SaveFile</a>                      |

**Configure a Mixer Measurement**

|                                        |                                     |                                  |
|----------------------------------------|-------------------------------------|----------------------------------|
| Calculate Input and Output frequencies | <a href="#">SENS:MIX:CALC</a>       | <a href="#">Calculate</a>        |
| Avoid Spurs                            | <a href="#">SENS:MIX:AVOIDspurs</a> | <a href="#">AvoidSpurs</a>       |
| X-axis display                         | <a href="#">CALC:MIX:XAXis</a>      | <a href="#">ActiveXAxisRange</a> |
| Apply mixer settings                   | <a href="#">SENS:MIX:APPLY</a>      | <a href="#">Apply</a>            |
| Number of Stages (1 or 2)              | <a href="#">SENS:MIX:STAG</a>       | <a href="#">LOStage</a>          |

**Set Input**

|                               |                                        |                                     |
|-------------------------------|----------------------------------------|-------------------------------------|
| Input start frequency         | <a href="#">SENS:MIX:INP:FREQ:STAR</a> | <a href="#">InputStartFrequency</a> |
| Input stop frequency          | <a href="#">SENS:MIX:INP:FREQ:STOP</a> | <a href="#">InputStopFrequency</a>  |
| Input power level             | <a href="#">SENS:MIX:INP:POW</a>       | <a href="#">InputPower</a>          |
| Numerator - Input Frac.Mult   | <a href="#">SENS:MIX:INP:FREQ:NUM</a>  | <a href="#">InputNumerator</a>      |
| Denominator - Input Frac.Mult | <a href="#">SENS:MIX:INP:FREQ:DEN</a>  | <a href="#">InputDenominator</a>    |


**Set LO**

|                                |                                        |                                      |
|--------------------------------|----------------------------------------|--------------------------------------|
| LO name                        | <a href="#">SENS:MIX:LO:NAME</a>       | <a href="#">LOName</a>               |
| LO sweep mode (fixed or swept) | <a href="#">SENS:MIX:LO:FREQ:MODE</a>  | <a href="#">LORangeMode</a>          |
| LO fixed frequency             | <a href="#">SENS:MIX:LO:FREQ:FIX</a>   | <a href="#">LOFixedFrequency</a>     |
| LO start frequency             | <a href="#">SENS:MIX:LO:FREQ:STARt</a> | <a href="#">LOStartFrequency</a>     |
| LO stop frequency              | <a href="#">SENS:MIX:LO:FREQ:STOP</a>  | <a href="#">LOStopFrequency</a>      |
| LO power                       | <a href="#">SENS:MIX:LO:POW</a>        | <a href="#">LOPower</a>              |
| Numerator - LO Frac.Mult       | <a href="#">SENS:MIX:LO:FREQ:NUM</a>   | <a href="#">LONumerator</a>          |
| Denominator - LO Frac.Mult     | <a href="#">SENS:MIX:LO:FREQ:DEN</a>   | <a href="#">LODenominator</a>        |
| Input Greater / Less than LO   | <a href="#">SENS:MIX:LO:FREQ:ILTI</a>  | <a href="#">IsInputGreaterThanLO</a> |

**Set IF**

|                            |                                       |                                  |
|----------------------------|---------------------------------------|----------------------------------|
| Sideband (high or low)     | <a href="#">SENS:MIX:IF:FREQ:SIDE</a> | <a href="#">IFSideband</a>       |
| IF start frequency         | <a href="#">SENS:MIX:IF:FREQ:STAR</a> | <a href="#">IFStartFrequency</a> |
| IF stop frequency          | <a href="#">SENS:MIX:IF:FREQ:STOP</a> | <a href="#">IFStopFrequency</a>  |
| Numerator - IF Frac.Mult   | <a href="#">SENS:MIX:IF:FREQ:NUM</a>  | <a href="#">IFNumerator</a>      |
| Denominator - IF Frac.Mult | <a href="#">SENS:MIX:IF:FREQ:DEN</a>  | <a href="#">IFDenominator</a>    |

**Set Output**

|                                                                                                        |                                  |                              |
|--------------------------------------------------------------------------------------------------------|----------------------------------|------------------------------|
|  deband (high or low) | <u>SENS:MIX:OUTP:FREQ:SIDE</u>   | <u>OutputSideband</u>        |
| Output start frequency                                                                                 | <u>SENS:MIX:OUTP:FREQ:STAR</u>   | <u>OutputStartFrequency</u>  |
| Output stop frequency                                                                                  | <u>SENS:MIX:OUTP:FREQ:STOP</u>   | <u>OutputStopFrequency</u>   |
| Output fixed frequency                                                                                 | <u>SENS:MIX:OUTP:FREQ:FIXed</u>  | <u>OutputFixedFrequency</u>  |
| <b>SMC (see <u>SCPI</u> and <u>COM</u> examples)</b>                                                   |                                  |                              |
| Create Cal object                                                                                      | None                             | <u>CreateCustomCal</u>       |
| Begin Cal                                                                                              | <u>SESS:INITiate</u>             | <u>Initialize</u>            |
| Sets to ECAL or Mechanical                                                                             | <u>SMC:TWOP:OPTion</u>           | <u>Do2PortEcal</u>           |
| Sets ECal module and characterization.                                                                 | <u>SESS:SMC:ECAL:CHAR</u>        | <u>ECALCharacterization</u>  |
| Sets ECal THRU method                                                                                  | <u>SESS:SMC:TWOP:METHOD</u>      | <u>ThruCalMethod</u>         |
| Sets ECAL auto-orientation ON or OFF                                                                   | <u>SESS:SMC:TWOP:ECAL:ORI</u>    | <u>AutoOrient</u>            |
| Sets ECAL port map when orientation is off.                                                            | <u>SESS:SMC:TWOP:ECAL:PORT</u>   | <u>EcalOrientation</u>       |
| Select either omit or perform Isolation                                                                | <u>SESS:SMC:TWOP:OMIT</u>        | <u>OmitIsolation</u>         |
| Sets the source port for the power calibration.                                                        | <u>SESS:SMC:PWRC:SRCPort</u>     | <u>CalibrationPort</u>       |
| Set connector type for each port                                                                       | <u>SESS:CONN:PORT:SEL</u>        | <u>ConnectorType</u>         |
| Set Cal Kit for the each port                                                                          | <u>SESS:CKIT:PORT:SEL</u>        | <u>CalKitType</u>            |
| Returns the number of steps required by the Calibration                                                | <u>SESS:STEPs?</u>               | <u>GenerateSteps</u>         |
| Returns the step description.                                                                          | <u>SESS:DESC?</u>                | <u>GetStepDescription</u>    |
| Acquire a calibration measurement.                                                                     | <u>SESS:ACQ</u>                  | <u>AcquireStep</u>           |
| Ends the calibration                                                                                   | <u>SESS:DONE</u>                 |                              |
| Generate Error Terms                                                                                   | <u>SESS:SAVE</u>                 | <u>GenerateErrorTerms</u>    |
| <b>VMC (see <u>SCPI</u> and <u>COM</u> examples)</b>                                                   |                                  |                              |
| Create Cal object                                                                                      | None                             | <u>CreateCustomCal</u>       |
| Begin Cal                                                                                              | <u>SESS:INITiate</u>             | <u>Initialize</u>            |
| Perform calibration or mixer characterization                                                          | <u>SESS:VMC:OPERation</u>        | <u>CharacterizeMixerOnly</u> |
| Specify direction of mixer characterization                                                            | <u>SESS:VMC:MIX:CHAR:CAL:REV</u> | <u>CharMixerReverse</u>      |
| Sets the <b>Mixer characterization</b> to ECal or Mech.                                                | <u>SESS:VMC:MIX:CHAR:CAL:OPT</u> | <u>Do1PortEcal</u>           |
| Sets ECAL auto-orientation ON or OFF                                                                   | <u>SESS:VMC:TWOP:ECAL:ORI</u>    | <u>AutoOrient Property</u>   |
| Set filename of mixer characterization file                                                            | <u>SESS:VMC:MIX:CHAR:CAL:FIL</u> | <u>CharFileName</u>          |
| Select ECal module and characterization to be used for mixer characterization                          | <u>SESS:VMC:MIX:ECAL:CHAR</u>    | <u>ECALCharacterization</u>  |
| Sets the port mapping for the mixer characterization.                                                  | <u>SESS:VMC:MIX:ECAL:PORT</u>    | <u>EcalOrientation1Port</u>  |

|                                                                        |                                |                             |
|------------------------------------------------------------------------|--------------------------------|-----------------------------|
| Sets the <b>2-Port calibration</b> to ECal or Mech.                    | <u>SESS:VMC:TWOP:OPTion</u>    | <u>Do2PortEcal</u>          |
| Select ECal module and characterization to be used for the calibration | <u>SESS:VMC:TWOP:ECAL:CHAR</u> | <u>ECALCharacterization</u> |
| Sets ECal method for performing the thru measurement                   | <u>SESS:VMC:TWOP:METH</u>      | <u>ThruCalMethod</u>        |
| Sets the port mapping for the calibration.                             | <u>SESS:VMC:TWOP:ECAL:PORT</u> | <u>EcalOrientation2Port</u> |
| Select either omit or perform Isolation                                | <u>SESS:VMC:TWOP:OMIT</u>      | <u>OmitIsolation</u>        |
| Set connector type for each port                                       | <u>SESS:CONN:PORT:SEL</u>      | <u>ConnectorType</u>        |
| Set Cal Kit for the each port                                          | <u>SESS:CKIT:PORT:SEL</u>      | <u>CalKitType</u>           |
| Returns the number of steps required by the Calibration                | <u>SESS:STEPS?</u>             | <u>GenerateSteps</u>        |
| Returns the step description.                                          | <u>SESS:DESC?</u>              | <u>GetStepDescription</u>   |
| Acquire a calibration measurement.                                     | <u>SESS:ACQ</u>                | <u>AcquireStep</u>          |
| Ends the calibration                                                   | <u>SESS:DONE</u>               |                             |
| Generate Error Terms                                                   | <u>SESS:SAVE</u>               | <u>GenerateErrorTerms</u>   |

## New Programming Commands

The following are new programming commands for **PNA release 5.25**: [Learn More](#)

| Description                                | SCPI                                        | COM                                          |
|--------------------------------------------|---------------------------------------------|----------------------------------------------|
| <b>Single-ended Measurements Fixturing</b> |                                             |                                              |
| Port Z Imaginary value.                    | <u>CALC:FSIM:SEND:ZCON:PORT:IMAG</u>        | <u>Fsim.PortArbzImag</u>                     |
| Port Z Real value.                         | <u>CALC:FSIM:SEND:ZCON:PORT:REAL</u>        | <u>FSim.PortArbzReal</u>                     |
| Port Z Real and Imaginary.                 | <u>CALC:FSIM:SEND:ZCON:PORT:Z0</u>          | <u>FSim.PortArbzZ0</u>                       |
| <b>Delta Match Cal</b>                     |                                             |                                              |
| Initiate Cal                               | <u>SENS:CORR:COLL:GUID:DMAT</u>             | <u>guid.GenerateGlobalDeltaMatchSequence</u> |
| Read ports that require Cal                | <u>SENS:CORR:COLL:GUID:DMAT:APPLY:PORT?</u> | <u>guid.PortsNeedingDeltaMatch</u>           |
| Apply a Cal                                | <u>SENS:CORR:COLL:GUID:DMAT:APPLY</u>       | <u>guid.ApplyDeltaMatchFromCalSet</u>        |

The following are new programming commands for **PNA release 5.22**: [Learn More](#)

| Description                                                  | SCPI                                | COM                              |
|--------------------------------------------------------------|-------------------------------------|----------------------------------|
| <b>Balanced Measurements Fixturing</b>                       |                                     |                                  |
| Sets imaginary value for common port impedance conversion.   | <u>CALC:FSIM:BAL:CZC:BPORt:IMAG</u> | <u>FSim.CmnModeZConvPortImag</u> |
| Sets real value for common port impedance conversion.        | <u>CALC:FSIM:BAL:CZC:BPORt:REAL</u> | <u>FSim.CmnModeZConvPortReal</u> |
| Sets impedance value for common port impedance conversion.   | <u>CALC:FSIM:BAL:CZC:BPORt:Z0:R</u> | <u>FSim.CmnModeZConvPortZ0</u>   |
| Turns ON/OFF common port impedance conversion.               | <u>CALC:FSIM:BAL:CZC:STATe</u>      | <u>FSim.CmnModeZConvState</u>    |
| Sets Capacitance value of the differential matching circuit. | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:C</u> | <u>FSim.DiffPortMatch_C</u>      |
| Sets Conductance value of the differential matching circuit. | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:G</u> | <u>FSim.DiffPortMatch_G</u>      |
| Sets Inductance value of the differential matching circuit.  | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:L</u> | <u>FSim.DiffPortMatch_L</u>      |

|                                                                                               |                                        |                                                                                      |
|-----------------------------------------------------------------------------------------------|----------------------------------------|--------------------------------------------------------------------------------------|
| Sets Resistance value of the differential matching circuit.                                   | <u>CALC:FSIM:BAL:DMC:BPOR:PAR:R</u>    | <u>FSim.DiffPortMatch_R</u>                                                          |
| Sets differential matching circuit type.                                                      | <u>CALC:FSIM:BAL:DMC:BPOR:TYPE</u>     | <u>FSim.DiffPortMatchMode</u>                                                        |
| Specifies the 2-port touchstone file for user-defined differential matching circuit is saved. | <u>CALC:FSIM:BAL:DMC:BPOR:USER:FIL</u> | <u>FSim.DiffPortMatchUserFilename</u>                                                |
| Turns ON/OFF differential matching circuit function.                                          | <u>CALC:FSIM:BAL:DMC:STATe</u>         | <u>FSim.DiffPortMatchState</u>                                                       |
| Sets imaginary value for differential port impedance conversion.                              | <u>CALC:FSIM:BAL:DZC:BPOR:IMAG</u>     | <u>FSim.DiffZConvPortImag</u>                                                        |
| Sets real value for differential port impedance conversion.                                   | <u>CALC:FSIM:BAL:DZC:BPOR:REAL</u>     | <u>FSim.DiffZConvPortReal</u>                                                        |
| Sets impedance value for differential port impedance conversion.                              | <u>CALC:FSIM:BAL:DZC:BPOR:Z0:R</u>     | <u>FSim.DiffZConvPortZ0</u>                                                          |
| Turns ON/OFF differential port impedance conversion.                                          | <u>CALC:FSIM:BAL:DZC:STATe</u>         | <u>FSim.DiffZConvState</u>                                                           |
| Specifies *.s4p filename.                                                                     | <u>CALC:FSIM:EMB:NETW:FIL</u>          | <u>FSim.Embed4PortNetworkFilename</u>                                                |
| Specify embed, de-embed, or none.                                                             | <u>CALC:FSIM:EMB:NETW:TYPE</u>         | <u>FSim.Embed4PortNetworkMode</u>                                                    |
| Turns ON or OFF 4-port Network Embed/De-embed                                                 | <u>CALC:FSIM:EMB:STAT</u>              | <u>FSim.Embed4PortState</u>                                                          |
| Specify All PNA Port connections                                                              |                                        | <u>Embed4PortList</u>                                                                |
| Read PNA Port connections for all topologies.                                                 |                                        | <u>Embed4PortA</u><br><u>Embed4PortB</u><br><u>Embed4PortC</u><br><u>Embed4PortD</u> |
| Specifies PNA port connections with topology A.                                               | <u>CALC:FSIM:EMB:TOP:A:PORT</u>        |                                                                                      |
| Specifies PNA port connections with topology B.                                               | <u>CALC:FSIM:EMB:TOP:B:PORT</u>        |                                                                                      |
| Specifies PNA port connections with topology C.                                               | <u>CALC:FSIM:EMB:TOP:C:PORT</u>        |                                                                                      |
| Specifies the PNA / DUT topology.                                                             | <u>CALC:FSIM:EMB:TYPE</u>              | <u>FSim.Embed4PortTopology</u>                                                       |

## Interface Control

|                          |                                |                 |
|--------------------------|--------------------------------|-----------------|
| Interface Control ON OFF | <u>Control:Interface:State</u> | <u>IC.State</u> |
|--------------------------|--------------------------------|-----------------|

Recall Interface Control file                      Control:Interface:Config                      IC.ConfigurationFile

## Calibrations

Turn Correction ON|OFF for a channel                      chan.ErrorCorrection

Perform receiver power cal                      DoReceiverPowerCal

## Automatic Port Extensions

Sets the frequencies used for calculation                      SENS:CORR:EXT:AUTO:CONFig                      AutoPortExtConfig

Include loss correction?                      SENS:CORR:EXT:AUTO:LOSS                      AutoPortExtLoss

Include DC Offset?                      SENS:CORR:EXT:AUTO:DcoF                      AutoPortExtDCOffset

Measure OPEN or SHORT.                      SENS:CORR:EXT:AUTO:MEASure                      AutoPortExtMeasure

Enable specified port.                      SENS:CORR:EXT:AUTO:PORT<n>                      AutoPortExtState

Clears old port extension delay and loss data.                      SENS:CORR:EXT:AUTO:RESet                      AutoPortExtReset

Set user span start frequency.                      SENS:CORR:EXT:AUTO:STARt                      AutoPortExtSearchStart

Set user span stop frequency.                      SENS:CORR:EXT:AUTO:STOP                      AutoPortExtSearchStop

## E5091A Test Set Control

Reads the number of ports                      SENS:MULT:COUN?                      e5091.NumberOfPorts

Turns ON and OFF the property display                      SENS:MULT1:DISP                      e5091.ShowProperties

Sets the control lines of the specified E5091A                      SENS:MULT1:TSET:OUTP                      e5091.ControlLines

Switches Port 1                      SENS:MULT:TSET9:PORT1                      e5091.OutputPort

Switches Port 2                      SENS:MULT:TSET9:PORT2                      e5091.OutputPort

Switches Port 3                      SENS:MULT:TSET9:PORT3                      e5091.OutputPort

Switches Port 4                      SENS:MULT:TSET9:PORT4                      e5091.OutputPort

Turns ON/OFF switching.                      SENS:MULT:STATe                      e5091.Enabled

Return ID of the testset                      N/A                      ID Property

## User Preset

User Preset                      SYST:UPReset                      UserPreset



|                                    |                            |                            |
|------------------------------------|----------------------------|----------------------------|
| Load User Preset file              | <u>SYST:UPReset:LOAD</u>   | <u>UserPresetLoadFile</u>  |
| Save Current state as User Preset  | <u>SYST:UPReset:SAVE</u>   | <u>UserPresetSaveState</u> |
| Enable Front Panel for User Preset | <u>SYST:UPReset:FPANel</u> | <u>UserPresetEnable</u>    |

### Miscellaneous

|                                                                      |                            |     |
|----------------------------------------------------------------------|----------------------------|-----|
| Transfers data between the PNA and an external controller using GPIB | <u>MMEMory:TRANsfer</u>    | N/A |
| Sets the internal state of the selected ECAL module.                 | <u>CONT:ECAL:MOD:STATe</u> | N/A |

The following are new programming commands for **PNA release 5.0**: [Learn More](#)

| Description                                                 | SCPI                              | COM                              |
|-------------------------------------------------------------|-----------------------------------|----------------------------------|
| <b>Material and Aux IO Capabilities</b>                     |                                   |                                  |
| Sets trigger delay for a channel                            | <u>SENS:SWE:TRIG:DEL</u>          | <u>ExternalTriggerDelay</u>      |
| Controls Mat Handler Connector pin 21 (ready for trigger).  | <u>CONT:HAND:RTR:STAT</u>         | <u>ReadyForTriggerState</u>      |
| Controls Mat Handler Connector pin 20 (index signal).       | <u>CONT:HAND:IND:STAT</u>         | <u>matHand.IndexState</u>        |
| Returns the most recent Mat Handler pass/fail status value. | <u>CONT:HAND:PASSfail:STATus?</u> | <u>object.PassFailStatus</u>     |
| Sets the Mat Handler pass/fail policy.                      | <u>CONT:HAND:PASSfail:POLicy</u>  | <u>object.PassFailPolicy</u>     |
| Returns the most recent Aux IO pass/fail status value.      | <u>CONT:AUX:PASSfail:STATus?</u>  | <u>object.PassFailStatus</u>     |
| Sets the Aux IO Pass/Fail policy.                           | <u>CONT:AUX:PASSfail:POLicy</u>   | <u>object.PassFailPolicy</u>     |
| Shows or Hides Pass/Fail dialog box.                        | <u>DISP:FSIGN</u>                 | <u>app.DisplayGlobalPassFail</u> |
| <b>Data Trace Offset</b>                                    |                                   |                                  |
| Phase Offset                                                | <u>CALC:OFFS:PHASe</u>            | <u>meas.PhaseOffset</u>          |
| Magnitude Offset                                            | <u>CALC:OFFS:MAGN</u>             | <u>meas.MagnitudeOffset</u>      |
| Magnitude Slope Offset                                      | <u>CALC:OFFS:MAGN:SLOP</u>        | <u>meas.MagnitudeSlopeOffset</u> |

## Balanced Measurements

Balanced measurement settings      Calc:FSIMulator      BalancedMeasurement Object

Topology settings      Calc:FSIMulator      BalancedTopology Object

## Port Ext. and Fixturing

Set Freq 1|2      SENS:CORR:EXT:PORT:FREQ      Fix.PortFreq1

Set Loss 1|2      SENS:CORR:EXT:PORT:LOSS      fix.PortLoss1

Use 1|2      SENS:CORR:EXT:PORT:INCL      fix.PortExtUse1

All fixturing commands      Calc:FSIMulator      Fixturing Object

## Calibrations

Receiver Power Cal Offset      SENS:CORR:RPOW:OFFS

Perform a Guided Cal using COM      GuidedCal Object

Create new Cal Set      SENS:CORR:CSET:CREate

Set/change name of new Cal Set      SENS:CORR:CSET:NAME

Read/Write Cal Set data      SENS:CORR:CSET:DATA

Automatically save User Cal Set      SENS:CORR:PREF:CSET:SAVU

Set port pairs for Guided Cal THRU      SENS:CORR:COLL:GUID:THRU:PORT      ThruCalMethod


## Miscellaneous

Executes a statistical analysis      CALC:FUNC:EXEC

---

The following are new programming commands for **PNA release 4.2:**

| Description                                           | SCPI                               | COM                             |
|-------------------------------------------------------|------------------------------------|---------------------------------|
| <b>GPIB Pass Through</b>                              |                                    |                                 |
| Open a GPIB pass-through session                      | <u>SYST:COMM:GPIB:RDEV:OPEN</u>    | N/A                             |
| Write commands to the GPIB pass-through device.       | <u>SYST:COMM:GPIB:RDEV:WRIT</u>    | N/A                             |
| Reads string data from the GPIB pass-through device.  | <u>SYST:COMM:GPIB:RDEV:READ?</u>   | N/A                             |
| Closes a GPIB pass-through session                    | <u>SYST:COMM:GPIB:RDEV:CLOS</u>    | N/A                             |
| Closes ALL GPIB pass-through sessions                 | <u>SYST:COMM:GPIB:RDEV:RES</u>     | N/A                             |
| Writes data (without header) to a pass-through device | <u>SYST:COMM:GPIB:RDEV:WBINary</u> | N/A                             |
| Writes data (with header) to a pass-through device    | <u>SYST:COMM:GPIB:RDEV:WBLock:</u> | N/A                             |
| <b>Time Domain Coupling / Distance Markers</b>        |                                    |                                 |
| Enable trace coupling                                 | <u>SENS:COUP:PAR</u>               | <u>CoupleChannelParams</u>      |
| Set gate coupling parameters                          | <u>CALC:FILT:COUP:PAR</u>          | <u>CoupledParameters</u>        |
| Set transform coupling parameters                     | <u>CALC:TRAN:COUP:PAR</u>          | <u>CoupledParameters</u>        |
| Specify measurement type for distance markers         | <u>CALC:TRAN:TIME:MARK:MODE</u>    | <u>DistanceMarkerMode</u>       |
| Specify units for distance markers                    | <u>CALC:TRAN:TIME:MARK:UNIT</u>    | <u>DistanceMarkerUnit</u>       |
| Set and return marker distance value                  | <u>CALC:MARK:DIST</u>              | <u>Distance</u>                 |
| <b>Miscellaneous</b>                                  |                                    |                                 |
| Accept trigger before armed                           | <u>CONT:SIGN:TRIG:ATBA</u>         | <u>AcceptTriggerBeforeArmed</u> |
| Output trigger enable                                 | <u>CONT:SIGN:TRIG:OUTP</u>         | <u>TriggerOutputEnabled</u>     |
| Set display window size                               | <u>DISPlay:WINDow:SIZE</u>         |                                 |
| Allow arbitrary segments                              | <u>SENS:SEGM:ARB</u>               | <u>AllowArbitrarySegments</u>   |
| Configure Pulsed App .dll                             | <u>ConfigNarrowBand2 Method</u>    | <u>ConfigNarrowBand2 Method</u> |

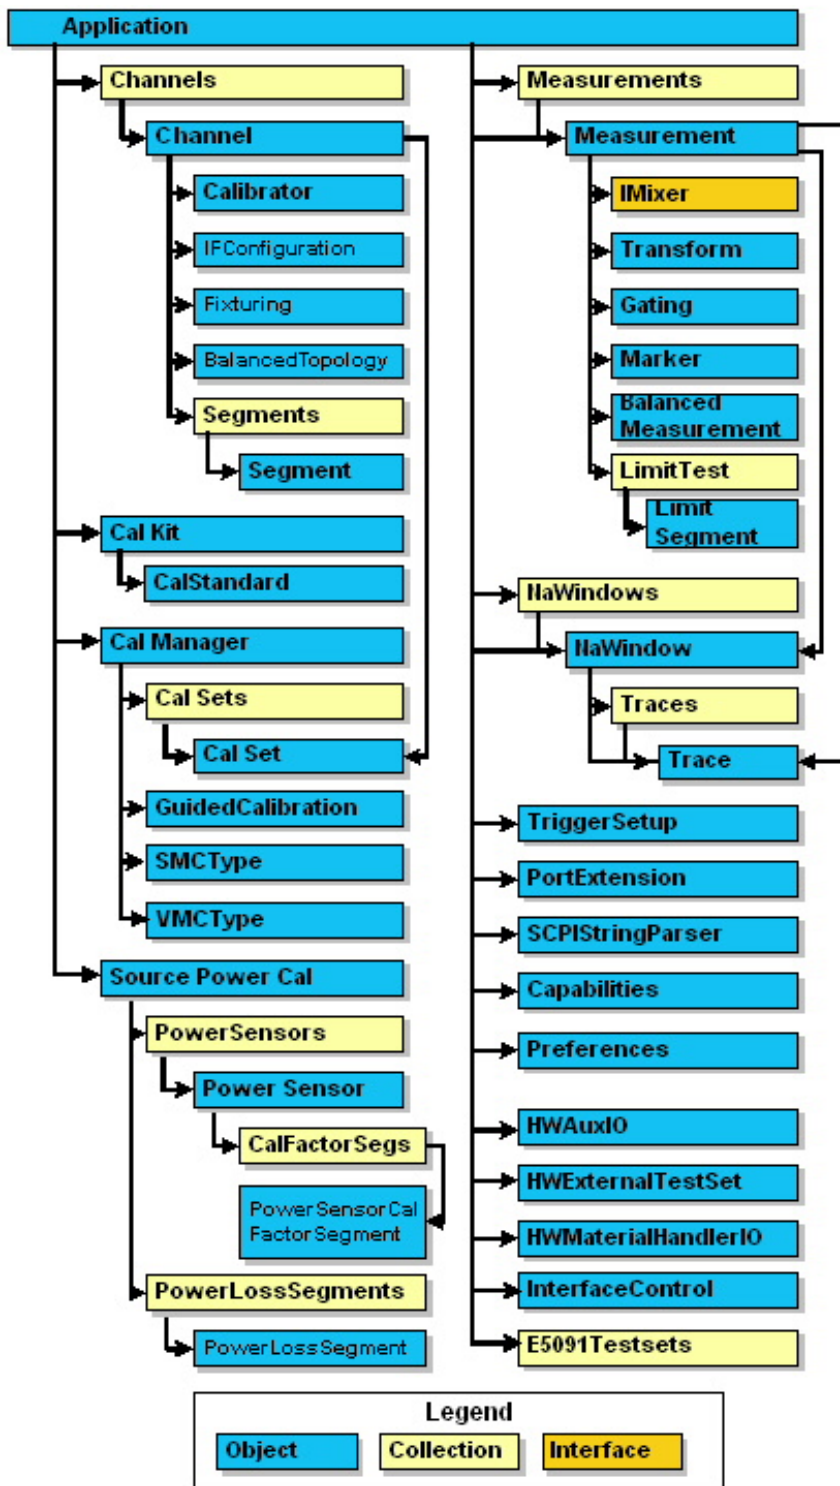

## Programming Guide

---



### **Command Search by Function**

COM and SCPI commands grouped like the PNA display menu.

| GPIB / SCPI                                | COM                                       |
|--------------------------------------------|-------------------------------------------|
| <a href="#"><u>Command Tree</u></a>        | <a href="#"><u>COM Object Model</u></a>   |
| <a href="#"><u>Example Programs</u></a>    | <a href="#"><u>Example Programs</u></a>   |
| <a href="#"><u>Learning about GPIB</u></a> | <a href="#"><u>Learning about COM</u></a> |

- [New Programming Commands](#)
- [New Code Translator App.](#)
- [Obsolete / Replacement Commands](#)
- [Data Access Map](#)
- See more PNA programming information and examples at: <http://na.tm.agilent.com/pna/programming/>

## Obsolete / Replacement Commands

---

As we expand the capability of the PNA, we will continue to develop new commands. Some of these new commands replace an existing command, giving it more functionality. Although the existing command will continue to work as usual, we recommend using the new command in code that you develop.

See [SCPI Replacement Commands](#).

### COM Replacement Commands

| Obsolete Command                                    | Replacement Command                                   |
|-----------------------------------------------------|-------------------------------------------------------|
| <a href="#">Acquire Cal Standard Method</a>         | <a href="#">Acquire Cal Standard2 Method</a>          |
| <a href="#">Create SParameter Method</a>            | <a href="#">Create SParameterEX Method</a>            |
| <a href="#">CreateCustomMeasurement Method</a>      | <a href="#">CreateCustomMeasurementEx Method</a>      |
| <a href="#">Calibrator.getErrorTerm</a>             | <a href="#">GetErrorTermByString_Method</a>           |
| <a href="#">Calibrator.getStandard</a>              | <a href="#">GetStandardByString_Method</a>            |
| <a href="#">Calibrator.putErrorTerm</a>             | <a href="#">PutErrorTermByString_Method</a>           |
| <a href="#">Calibrator.putStandard</a>              | <a href="#">PutStandardByString_Method</a>            |
| <a href="#">AcquireCalConfidenceCheckECAL</a>       | <a href="#">AcquireCalConfidenceCheckECALEX</a>       |
| <a href="#">DoECAL1Port Method</a>                  | <a href="#">DoECAL1PortEx Method</a>                  |
| <a href="#">DoECAL2Port Method</a>                  | <a href="#">DoECAL2PortEx Method</a>                  |
| <a href="#">ECALCharacterization Property</a>       | <a href="#">ECALCharacterizationEx Property</a>       |
| <a href="#">ECALPortMap_Property</a>                | <a href="#">ECALPortMapEx_Property</a>                |
| <a href="#">Get ECAL Module Info Method</a>         | <a href="#">Get ECALModuleInfoEx Method</a>           |
| <a href="#">IsECALModuleFound Property</a>          | <a href="#">IsECALModuleFoundEx Property</a>          |
| <a href="#">Trigger Signal Property</a>             | <a href="#">Source Property</a>                       |
| <a href="#">Trigger Type Property</a>               | <a href="#">Scope Property</a>                        |
| <a href="#">get SourcePowerCalData Method</a>       | <a href="#">Get SourcePowerCalDataEx Method</a>       |
| <a href="#">get SourcePowerCalDataScalar Method</a> | <a href="#">Get SourcePowerCalDataScalarEx Method</a> |
| <a href="#">put SourcePowerCalData Method</a>       | <a href="#">Put SourcePowerCalDataEx Method</a>       |
| <a href="#">put SourcePowerCalDataScalar Method</a> | <a href="#">Put SourcePowerCalDataScalarEx Method</a> |
| <a href="#">ConfigNarrowBand Method</a>             | <a href="#">ConfigNarrowBand2 Method</a>              |
| <a href="#">ConfigNarrowBand2 Method</a>            | <a href="#">ConfigNarrowBand3 Method</a>              |

|                                          |                                           |
|------------------------------------------|-------------------------------------------|
| <u>StandardForClass Property</u>         | <u>GetStandardForClass Method</u>         |
|                                          | <u>SetStandardForClass Method</u>         |
| <u>Input A Property</u>                  | No replacement                            |
| <u>Input B Property</u>                  | No replacement                            |
| <u>Input C Property</u>                  | No replacement                            |
| <u>Port 1 Property</u>                   | <u>PortDelay Property</u>                 |
| <u>Port 2 Property</u>                   | <u>PortDelay Property</u>                 |
| <u>Port 3 Property</u>                   | <u>PortDelay Property</u>                 |
| <u>Normalization Property</u>            | <u>Error Correction Property</u>          |
| <u>InterpolateNormalization Property</u> | <u>Interpolate Correction Property</u>    |
| <u>Get ErrorTermComplex2 Method</u>      | <u>GetErrorTermComplexByString Method</u> |
| <u>Get ErrorTermList Method</u>          | <u>GetErrorTermList2 Method</u>           |
| <u>Get Standard Complex Method</u>       | <u>GetStandardComplexByString Method</u>  |
| <u>Put ErrorTermComplex2 Method</u>      | <u>PutErrorTermComplexByString Method</u> |
| <u>Put Standard Complex Method</u>       | <u>PutStandardComplexByString Method</u>  |
| <u>Get ErrorTerm2 Method</u>             | <u>GetErrorTermByString Method</u>        |
| <u>Get Standard2 Method</u>              | <u>Get StandardByString Method</u>        |
| <u>Get StandardsList Method</u>          | <u>Get StandardList2 Method</u>           |
| <u>Put ErrorTerm2 Method</u>             | <u>PutErrorTermByString Method</u>        |
| <u>Put Standard2 Method</u>              | <u>PutStandardByString Method</u>         |
| <u>ECALIsolation Property</u>            | No replacement                            |
| <u>DataToDivisor</u>                     | <u>DoReceiverPowerCal Method</u>          |
| <u>LogMagnitudeOffset</u>                |                                           |
| <u>Normalization</u>                     |                                           |
| <u>InterpolateNormalization</u>          |                                           |

## SCPI Replacement Commands

|                                 |                            |
|---------------------------------|----------------------------|
| <u>TRIGger[:SEQuence]:LEVel</u> | <u>CONTRol:SIGNal</u>      |
| <u>DISPlay:TILE</u>             | <u>DISP:ARRange</u>        |
| <u>CALC:CORR:OFFS:MAGN</u>      | <u>SENS:CORR:RPOW:OFFS</u> |
| <u>CALC:NORM</u>                | <u>SENS:CORR:COLL:METH</u> |
|                                 | <u>SENS:CORR:COLL</u>      |
| <u>CALC:NORM:STAT</u>           | <u>SENS:CORR</u>           |
| <u>CALC:NORM:INT</u>            | <u>SENS:CORR:INT</u>       |
| <u>SENS:CORR:EXT:REC</u>        | No replacement             |
| <u>SENS:CORR:ISOLation</u>      | No replacement             |



|                        |                              |                                  |
|------------------------|------------------------------|----------------------------------|
| AutoScale              | <u>DISP:WIND:TRAC:Y:AUTO</u> | <u>Trce.Autoscale</u>            |
| AutoScale All          | None                         | <u>Trce.Autoscale</u>            |
| Per Division           | <u>DISP:WIND:TRAC:Y:PDIV</u> | <u>trce.YScale</u>               |
| Reference Level        | <u>DISP:WIND:TRAC:Y:RLEV</u> | <u>trce.ReferenceValue</u>       |
| Reference Position     | <u>DISP:WIND:TRAC:Y:RPOS</u> | <u>trce.ReferencePosition</u>    |
| Electrical Delay       | <u>CALC:CORR:EDEL:TIME</u>   | <u>meas.ElectricalDelay</u>      |
| Phase Offset           | <u>CALC:OFFS:PHAS</u>        | <u>meas.PhaseOffset</u>          |
| Magnitude Offset       | <u>CALC:OFFS:MAGN</u>        | <u>meas.MagnitudeOffset</u>      |
| Magnitude Slope Offset | <u>CALC:OFFS:MAGN:SLOP</u>   | <u>meas.MagnitudeSlopeOffset</u> |

**Power | Segment | Trigger**

|                                                                                                              |                            |                                    |
|--------------------------------------------------------------------------------------------------------------|----------------------------|------------------------------------|
| Sweep Time Value                                                                                             | <u>SENS:SWE:TIME:AUTO</u>  | <u>chan.SweepTime</u>              |
| IF Bandwidth                                                                                                 | <u>SENS:BWID</u>           | <u>chan.IFBandwidth</u>            |
| Previous IF Bandwidth                                                                                        | None                       | <u>chan.Previous_IFBandwidth</u>   |
| Next IFBandwidth                                                                                             | None                       | <u>chan.Next_IFBandwidth</u>       |
| Reduce IF BW                                                                                                 | <u>SENS:BWID:TRACK</u>     | <u>chan.ReduceIFBW</u>             |
| Number of Points                                                                                             | <u>SENS:SWE:POIN</u>       | <u>chan.NumberOfPoints</u>         |
| Sweep Type (Lin   Pwr   CW   Seg)                                                                            | <u>SENS:SWE:TYPE</u>       | <u>chan.SweepType</u>              |
| Sweep Generation (Stepped   Analog)                                                                          | <u>SENS:SWE:GEN</u>        | <u>chan.SweepGenerationMode</u>    |
| Dwell Time Value                                                                                             | <u>SENS:SWE:DWEL</u>       | <u>chan.DwellTime</u>              |
| Alternate Sweeps                                                                                             | <u>SENS:COUP</u>           | <u>chan.AlternateSweep</u>         |
| External ALC                                                                                                 | <u>SOUR:POW:DET</u>        | <u>app.ExternalALC</u>             |
| <b>Power Sweep</b>                                                                                           |                            |                                    |
| Start Power                                                                                                  | <u>SOUR:POW:STAR</u>       | <u>chan.StartPower</u>             |
| Stop Power                                                                                                   | <u>SOUR:POW:STOP</u>       | <u>chan.StopPower</u>              |
| Center                                                                                                       | <u>SOUR:POW:CENT</u>       |                                    |
| Span                                                                                                         | <u>SOUR:POW:SPAN</u>       |                                    |
| <b>Segment Sweep</b>                                                                                         |                            |                                    |
| ON OFF                                                                                                       | <u>SENS:SEGM</u>           | <u>Seg.State</u>                   |
| Add a segment                                                                                                | <u>SENS:SEGM:ADD</u>       | <u>Segs.Add</u>                    |
| Delete a segment                                                                                             | <u>SENS:SEGM:DEL</u>       | <u>segments.Remove</u>             |
| Delete all segments                                                                                          | <u>SENS:SEGM:DEL:ALL</u>   | None                               |
| Count the segments                                                                                           | <u>SENS:SEGM:COUN</u>      | <u>chans.Count</u>                 |
| Read the segment number                                                                                      | None                       | <u>seg.SegmentNumber</u>           |
|  Segment Center Frequency | <u>SENS:SEGM:FREQ:CENT</u> | <u>chan.centerFrequency</u>        |
| Segment Frequency Span                                                                                       | <u>SENS:SEGM:FREQ:SPAN</u> | <u>chan.FrequencySpan</u>          |
| Segment Start Frequency                                                                                      | <u>SENS:SEGM:FREQ:STAR</u> | <u>Chan.StartFrequency</u>         |
| Segment Stop Frequency                                                                                       | <u>SENS:SEGM:FREQ:STOP</u> | <u>Chan.StopFrequency</u>          |
| Number of Points                                                                                             | <u>SENS:SEGM:SWE:POIN</u>  | <u>seg.NumberOfPoints</u>          |
| IF Bandwidth                                                                                                 | <u>SENS:SEGM:BWID</u>      | <u>seg.IFBandwidth</u>             |
| IF Bandwidth Option                                                                                          | <u>SENS:SEGM:BWID:CONT</u> | <u>segs.IFBandwidthOption</u>      |
| Source Power                                                                                                 | <u>SENS:SEGM:POW</u>       | <u>chan.TestPortPower</u>          |
| Source Power Option                                                                                          | <u>SENS:SEGM:POW:CONT</u>  | <u>segs.SourcePowerOption</u>      |
| X-Axis Point Spacing                                                                                         | <u>SENS:SEGM:X:SPAC</u>    | <u>chan.XAxisPointSpacing</u>      |
| Allow Arbitrary Segments                                                                                     | <u>SENS:SEGM:ARB</u>       | <u>segs.AllowArbitrarySegments</u> |
| Upload a segment table                                                                                       | None                       | <u>SetAllSegmernts</u>             |

| <b>Trigger</b>                                                 |                                |                                          |
|----------------------------------------------------------------|--------------------------------|------------------------------------------|
| <b>Source</b> (where trigger comes from)                       |                                |                                          |
| Source (Int   Ext   Manual)                                    | <u>TRIG:SOUR</u>               | <u>trigSetup.Source</u>                  |
| Internal   Manual                                              | <u>INIT:CONT</u>               |                                          |
| Trigger! (for Manual Source)                                   | <u>INIT</u>                    | <u>app.ManualTrigger</u>                 |
| <b>Scope</b> (what is triggered)                               |                                |                                          |
| Scope (Global   Channel)                                       | <u>TRIG:SCOP</u>               | <u>trigSetup.Scope</u>                   |
| <b>Channel Settings</b> (how the channel responds to triggers) |                                |                                          |
| Continuous                                                     | <u>SENS:SWE:MODE CONTInous</u> | <u>chan.Continuous</u>                   |
| Read Continuous Mode                                           |                                | <u>chan.IsContinuous</u>                 |
| Number of Groups                                               | <u>SENS:SWE:GRO:COUN</u>       | <u>chan.NumberOfGroups</u>               |
| Read Groups                                                    |                                | <u>chan.GetNumberOfGroups</u>            |
| Hold                                                           | <u>SENS:SWE:MODE HOLD</u>      | <u>chan.Hold</u>                         |
| Hold Mode (read-only)                                          |                                | <u>chan.IsHold</u>                       |
| All channels in Hold                                           | <u>SYST:CHAN:HOLD</u>          | <u>chans.Hold</u>                        |
| All channels Resume                                            | <u>SYST:CHAN:RESume</u>        | <u>chans.Resume</u>                      |
| Single                                                         | <u>SENS:SWE:GRO:COUN 1</u>     | <u>chan.Single</u>                       |
| Trigger Mode (Point   Measurement)                             | <u>SENS:SWE:TRIG:POIN</u>      | <u>chan.TriggerMode</u>                  |
| Restart                                                        | <u>INIT</u>                    |                                          |
| Abort                                                          | <u>ABOR</u>                    | <u>chan.Abort</u>                        |
| <b>External Trigger</b>                                        |                                |                                          |
| External Trigger Behavior                                      | <u>CONT:SIGNal</u>             | <u>ExternalTriggerConnectionBehavior</u> |
| Trigger Delay (Global)                                         | <u>TRIG:DEL</u>                | <u>app.TriggerDelay</u>                  |
| Trigger Delay (Channel)                                        | <u>SENS:SWE:TRIG:DEL</u>       | <u>chan.ExternalTriggerDelay</u>         |
| Accept Trigger Before Armed                                    | <u>CONT:SIGN:TRIG:ATBA</u>     | <u>AcceptTriggerBeforeArmed</u>          |
| Output trigger enable                                          | <u>CONT:SIGN:TRIG:OUTP</u>     | <u>TriggerOutputEnabled</u>              |

**User Preset | Status | Events | Macros | Rear Panel | Pass-through |**

|                                                      |                                 |                                |
|------------------------------------------------------|---------------------------------|--------------------------------|
| Frequency Blanking                                   | <u>SEC:LEVel</u>                | <u>app.SecurityLevel</u>       |
| Local Lockout                                        | <u>Local Lockout</u>            | <u>app.LocalLockoutState</u>   |
| Preset                                               | <u>SYST:PRES</u><br><u>*RST</u> | <u>app.Preset</u>              |
| Preset plus delete window                            | <u>SYST:FPRreset</u>            | <u>app.Reset</u>               |
| Return Full computer name                            |                                 | <u>app.SystemName</u>          |
| Set and return GPIB address                          |                                 | <u>app.GPIBAddress</u>         |
| Set PNA to GPIB system controller or talker/listener |                                 | <u>app.GPIBMode</u>            |
| Set and return SICL address                          |                                 | <u>app.SICLAddress</u>         |
| Control the PNA via SICL                             |                                 | <u>app.SICL</u>                |
| Quit application                                     |                                 | <u>app.Quit</u>                |
| System Impedance                                     | <u>SENS:CORR:IMP:INP:MAGN</u>   | <u>SystemImpedanceZ0</u>       |
| <b>User Preset</b>                                   |                                 |                                |
| User Preset                                          | <u>SYST:UPReset</u>             | <u>app.UserPreset</u>          |
| Load User Preset file                                | <u>SYST:UPReset:LOAD</u>        | <u>app.UserPresetLoadFile</u>  |
| Save Current state as User Preset                    | <u>SYST:UPReset:SAVE</u>        | <u>app.UserPresetSaveState</u> |
| Enable Front Panel for User Preset                   | <u>SYST:UPReset:FPANel</u>      | <u>app.UserPresetEnable</u>    |
| <b>Status Commands</b>                               |                                 |                                |
| Status Registers                                     | <u>GP-IB&gt;Status</u>          |                                |
| *OPC;*WAI                                            | <u>GP-IB/Common_Commands</u>    |                                |
| <b>Events</b>                                        |                                 |                                |
| AllowAllEvents Method                                |                                 | <u>app.AllowAllEvents</u>      |
| AllowEventCategory Method                            |                                 | <u>app.AllowEventCategory</u>  |
| AllowEventMessage Method                             |                                 | <u>app.AllowEventMessage</u>   |
| AllowEventSeverity Method                            |                                 | <u>app.AllowEventSeverity</u>  |
| DisallowAllEvents Method                             |                                 | <u>app.DisallowAllEvents</u>   |
| MessageText Method                                   |                                 | <u>app.MessageText</u>         |
| OnCalEvent                                           |                                 | <u>app.OnCalEvent</u>          |
| OnChannelEvent                                       |                                 | <u>app.OnChannelEvent</u>      |
| OnDisplayEvent                                       |                                 | <u>app.OnDisplayEvent</u>      |
| OnHardwareEvent                                      |                                 | <u>app.OnHardwareEvent</u>     |
| OnMeasurementEvent                                   |                                 | <u>app.OnMeasurementEvent</u>  |
| OnSCPIEvent                                          |                                 | <u>app.OnSCPIEvent</u>         |
| OnSystemEvent                                        |                                 | <u>app.OnSystemEvent</u>       |
| OnUserEvent                                          |                                 | <u>app.OnUserEvent</u>         |

|                                                              |                                                    |                                               |
|--------------------------------------------------------------|----------------------------------------------------|-----------------------------------------------|
| SetFailOnOverRange                                           |                                                    | <a href="#"><u>app.SetFailOnOverRange</u></a> |
| <b>Macros</b>                                                |                                                    |                                               |
| Execute Macro                                                |                                                    | <a href="#"><u>app.ExecuteShortcut</u></a>    |
| Get Macro                                                    |                                                    | <a href="#"><u>app.GetShortcut</u></a>        |
| Delete Macro                                                 |                                                    | <a href="#"><u>app.DeleteShortCut</u></a>     |
| Put Macro                                                    |                                                    | <a href="#"><u>app.PutShortcut</u></a>        |
| <b>Rear Panel Connector Controls</b>                         |                                                    |                                               |
| Material Handler I/O Connector                               | <a href="#"><u>GP-IB\Control</u></a>               | <a href="#"><u>MaterialHandler IO</u></a>     |
| Auxiliary IO Connector                                       | <a href="#"><u>GP-IB\Control</u></a>               | <a href="#"><u>Aux IO</u></a>                 |
| External Test Set Connector                                  | <a href="#"><u>GP-IB\Control</u></a>               | <a href="#"><u>External Test Set</u></a>      |
| <b>GPIB Pass Through</b>                                     |                                                    |                                               |
| Open a GPIB pass-through session                             | <a href="#"><u>SYST:COMM:GPIB:RDEV:OPEN</u></a>    |                                               |
| Write string data to the GPIB pass-through device.           | <a href="#"><u>SYST:COMM:GPIB:RDEV:WRIT</u></a>    |                                               |
| Write data to the GPIB pass-through device (with header).    | <a href="#"><u>SYST:COMM:GPIB:RDEV:WBLOCK</u></a>  |                                               |
| Write data to the GPIB pass-through device (without header). | <a href="#"><u>SYST:COMM:GPIB:RDEV:WBINARY</u></a> |                                               |
| Reads string data from the GPIB pass-through device.         | <a href="#"><u>SYST:COMM:GPIB:RDEV:READ?</u></a>   |                                               |
| Closes a GPIB pass-through session                           | <a href="#"><u>SYST:COMM:GPIB:RDEV:CLOS</u></a>    |                                               |
| Closes ALL GPIB pass-through sessions                        | <a href="#"><u>SYST:COMM:GPIB:RDEV:RES</u></a>     |                                               |


**Balanced Meas | Format | Math | Smooth | Stats | Limits | Transform | Global Pass Fail**

|                                            |                                         |                                            |
|--------------------------------------------|-----------------------------------------|--------------------------------------------|
| Create S-Parameter Meas.                   |                                         | <a href="#">app.CreateSParameter</a>       |
| Create Measurement                         | <a href="#">CALC:PAR:DEF</a>            | <a href="#">app.CreateMeasurement</a>      |
| Add Measurement                            |                                         | <a href="#">meas.Add</a>                   |
| List Measurements                          | <a href="#">CALC:PAR:CAT</a>            |                                            |
| Delete a measurement                       | <a href="#">CALC:PAR:DEL</a>            | <a href="#">Measurements.Remove</a>        |
| Delete ALL measurements                    | <a href="#">CALC:PAR:DEL:ALL</a>        |                                            |
| Get a handle to a Trace                    |                                         | <a href="#">win.ActiveTrace</a>            |
| Select a Measurement                       | <a href="#">CALC:PAR:SEL</a>            | <a href="#">app.ActiveMeasurement</a>      |
| Read Channel Number                        |                                         | <a href="#">chan.ChannelNumber</a>         |
| Read Number of Measurements                |                                         | <a href="#">chans.Count</a>                |
| Read Measurement Parameter                 |                                         | <a href="#">meas.Parameter</a>             |
| Set / Read Measurement Name                |                                         | <a href="#">meas.Name</a>                  |
| Read Measurement Number                    |                                         | <a href="#">meas.Number</a>                |
| Change Parameter                           | <a href="#">CALC:PAR:MOD</a>            | <a href="#">meas.ChangeParameter</a>       |
| Measurement Format                         | <a href="#">CALC:FORM</a>               | <a href="#">meas.Format</a>                |
| <b>Balanced Measurements and Fixturing</b> |                                         |                                            |
| Configure Topology                         | <a href="#">CALC:FSIM:BAL</a>           | <a href="#">BalancedTopology</a> Object    |
| Configure Balanced Measurement             | <a href="#">CALC:FSIM:BAL</a>           | <a href="#">BalancedMeasurement</a> Object |
| <b>Format</b>                              |                                         |                                            |
| Format trace                               | <a href="#">CALC:FORM</a>               | <a href="#">Format</a> Property            |
| <b>Math</b>                                |                                         |                                            |
| Data Trace ON OFF                          | <a href="#">DISP:WIND:TRAC</a>          | <a href="#">meas.View</a>                  |
| Memory Trace ON OFF                        | <a href="#">DISP:WIND:TRAC:MEM</a>      | <a href="#">meas.View</a>                  |
| Data =>Memory                              | <a href="#">CALC:MATH:MEM</a>           | <a href="#">meas.DataToMemory</a>          |
| Trace Math (Add Sub Mult Div)              | <a href="#">CALC:MATH:FUNC</a>          | <a href="#">meas.TraceMath</a>             |
| <b>Smoothing</b>                           |                                         |                                            |
| Smoothing ON OFF                           | <a href="#">CALC:SMO</a>                | <a href="#">meas.Smoothing</a>             |
| Smoothing Aperture                         | <a href="#">CALC:SMO:APER</a>           | <a href="#">meas.SmoothingAperture</a>     |
| Smoothing Points                           | <a href="#">CALC:SMO:POIN</a>           |                                            |
| <b>Statistics</b>                          |                                         |                                            |
| Statistics ON OFF                          | <a href="#">CALC:FUNC:STAT</a>          | <a href="#">meas.ShowStatistics</a>        |
| Statistics Range                           | <a href="#">CALC:FUNC:DOM:USER</a>      | <a href="#">meas.StatisticsRange</a>       |
| Domain Range Start                         | <a href="#">CALC:FUNC:DOM:USER:STAR</a> | <a href="#">chan.UserRangeMin</a>          |
| Domain Range Stop                          | <a href="#">CALC:FUNC:DOM:USER:STOP</a> | <a href="#">chan.UserRangeMax</a>          |

|                                                                |                                                                       |                                  |
|----------------------------------------------------------------|-----------------------------------------------------------------------|----------------------------------|
| Set Type (Pk-Pk StdDev Mean)                                   | <u>CALC:FUNC:TYPE</u>                                                 |                                  |
| Get All Statistics Data                                        | <u>CALC:FUNC:DATA</u>                                                 | <u>meas.GetFilterStatistics</u>  |
| Get Standard Deviation                                         |                                                                       | <u>meas.StandardDeviation</u>    |
| Get Mean                                                       |                                                                       | <u>meas.Mean</u>                 |
| Get Peak to Peak                                               |                                                                       | <u>meas.PeakToPeak</u>           |
| <b>Limit Lines</b>                                             |                                                                       |                                  |
| Display Lines ON OFF                                           | <u>CALC:LIM:DISP:STAT</u>                                             | <u>Limttest.LineDisplay</u>      |
| Fail Sound ON OFF                                              | <u>CALC:LIM:SOUN</u>                                                  | <u>Limttest.SoundOnFail</u>      |
| Testing ON OFF                                                 | <u>CALC:LIM:STAT</u>                                                  | <u>Trans.State</u>               |
| Limit Test Failed                                              |                                                                       | <u>meas.LimitTestFailed</u>      |
| Count Limit Lines                                              |                                                                       | <u>chans.Count</u>               |
| Read Test Results                                              | <u>GP-IB_Command_Finder\Status</u>                                    | <u>limts.GetTestResult</u>       |
| Make Limit Lines                                               | <u>CALC:LIM:DATA</u>                                                  |                                  |
| Limit Line Type (Max Min)                                      | <u>CALC:LIM:SEGM:TYPE</u>                                             | <u>limts.Type</u>                |
| Begin Stimulus                                                 | <u>CALC:LIM:SEGM:STIM:STAR</u>                                        | <u>limtseg.BeginStimulus</u>     |
| End Stimulus                                                   | <u>CALC:LIM:SEGM:AMPL:STOP</u>                                        | <u>limtseg.EndStimulus</u>       |
| Begin Response                                                 | <u>CALC:LIM:SEGM1:AMPL:STAR</u>                                       | <u>limtseg.BeginResponse</u>     |
| End Response                                                   | <u>CALC:LIM:SEGM1:AMPL:STOP</u>                                       | <u>limtseg.EndResponse</u>       |
| <b>Global Pass/Fail</b>                                        |                                                                       |                                  |
| Show / hide the pass/fail dialog.                              | <u>DISP:FSIG</u>                                                      | <u>app.DisplayGlobalPassFail</u> |
| Sets the policy used to compute the global pass/fail value.    | <u>CONT:HAND:PASSfail:POL</u><br><u>CONT:AUX:PASSfail:POL</u>         | <u>obj.PassFailPolicy</u>        |
| Reads the most recent pass/fail status value.                  | <u>CONT:HAND:PASSfail:STATus?</u><br><u>CONT:AUX:PASSfail:STATus?</u> | <u>obj.PassFailStatus</u>        |
| Sets the logic of the AuxIO PassFail line.                     | <u>CONT:HAND:PASS:LOGic</u><br><u>CONT:AUX:PASS:LOGic</u>             | <u>obj.PassFailLogic</u>         |
| Sets the default logical pass/fail state.                      | <u>CONT:HAND:PASS:MODE</u><br><u>CONT:AUX:PASS:MODE</u>               | <u>obj.PassFailMode</u>          |
| Sets the scope (Global or channel) of AuxIO pass/fail testing. | <u>CONT:HAND:PASS:SCOP</u><br><u>CONT:AUX:PASS:SCOP</u>               | <u>obj.PassFailScope</u>         |
| <b>Transform</b>                                               |                                                                       |                                  |
| Transform ON OFF                                               | <u>CALC:TRAN:TIME:STAT</u>                                            | <u>trans.State</u>               |
| Mode (LowPass, BandPass)                                       | <u>CALC:TRAN:TIME</u>                                                 | <u>trans.Mode</u>                |
| Start Time                                                     | <u>CALC:TRAN:TIME:STAR</u>                                            | <u>trans.Start</u>               |
| Stop Time                                                      | <u>CALC:TRAN:TIME:STOP</u>                                            | <u>trans.Stop</u>                |
| Center                                                         | <u>CALC:TRAN:TIME:CENT</u>                                            | <u>trans.Center</u>              |
| Span                                                           | <u>CALC:TRAN:TIME:SPAN</u>                                            | <u>trans.Span</u>                |
| Step Rise Time                                                 | <u>CALC:TRAN:TIME:STAR</u>                                            | <u>trans.StepRiseTime</u>        |

|                                               |                                 |                                  |
|-----------------------------------------------|---------------------------------|----------------------------------|
| Set Low Pass Frequency                        | <u>CALC:TRAN:TIME:LPFR</u>      | <u>trans.SetFrequencyLowPass</u> |
| Enable trace coupling                         | <u>SENS:COUP:PAR</u>            | <u>CoupleChannelParams</u>       |
| Set transform coupling parameters             | <u>CALC:TRAN:COUP:PAR</u>       | <u>trans.CoupledParameters</u>   |
| Specify measurement type for distance markers | <u>CALC:TRAN:TIME:MARK:MODE</u> | <u>trans.DistanceMarkerMode</u>  |
| Specify units for distance markers            | <u>CALC:TRAN:TIME:MARK:UNIT</u> | <u>trans.DistanceMarkerUnit</u>  |
| Set and return marker distance value          | <u>CALC:MARK:DIST</u>           | <u>mark.Distance</u>             |
| <b>Gating</b>                                 |                                 |                                  |
| ON OFF                                        | <u>CALC:FILT:TIME:STAT</u>      | <u>gate.State</u>                |
| Type (BandPass, Notch)                        | <u>CALC:FILT:TIME</u>           | <u>gate.Type</u>                 |
| Shape                                         | <u>CALC:FILT:GATE:TIME:SHAP</u> | <u>gat.Shape</u>                 |
| Start                                         | <u>CALC:FILT:TIME:STAR</u>      | <u>gate.Start</u>                |
| Stop                                          | <u>CALC:FILT:GATE:TIME:STOP</u> | <u>gate.Stop</u>                 |
| Center                                        | <u>CALC:FILT:GATE:TIME:CENT</u> | <u>gate.Center</u>               |
| Span                                          | <u>CALC:FILT:GATE:TIME:SPAN</u> | <u>gate.Span</u>                 |
| Set gate coupling parameters                  |                                 |                                  |
| <b>Window</b>                                 |                                 |                                  |
| Kaiser Beta                                   | <u>CALC:TRAN:TIME:KBES</u>      | <u>trans.KaiserBeta</u>          |
| Impulse Width                                 | <u>CALC:TRAN:TIME:IMP:WIDT</u>  | <u>trans.ImpulseWidth</u>        |



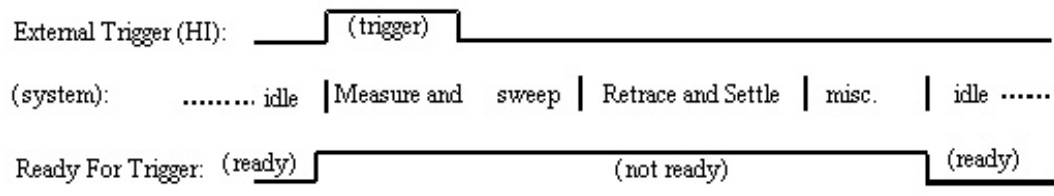


**Speed up Measurements !**

|                          |                         |                    |
|--------------------------|-------------------------|--------------------|
| Measurement Trace On Off | <u>DISP:WIND:TRAC</u>   | <u>meas.View</u>   |
| Display Update On Off    | <u>DISP:ENAB</u>        | None               |
| Window Update On Off     | <u>DISP:WIND:ENABLE</u> | None               |
| Analyzer Visible On Off  | None                    | <u>app.Visible</u> |


**Toolbars / Functions On|Off**

|                             |                                |                                    |
|-----------------------------|--------------------------------|------------------------------------|
| Status Bar On Off           | <u>DISP:ANN:STAT</u>           | <u>app.ShowStatusBar</u>           |
| Toolbars On Off             | None                           | <u>app.ShowToolbar</u>             |
| Tables On Off               | <u>DISP:WIND:TABLE</u>         | <u>win.ShowTable</u>               |
| Title Bars On Off           | None                           | <u>app.ShowTitleBars</u>           |
| X-axis values On Off        | <u>DISP:ANN:FREQ</u>           | <u>app.ShowStimulus</u>            |
| Marker Readout On Off       | <u>DISP:WIND:ANN:MARK:STAT</u> | <u>win.MarkerReadout</u>           |
| Trace Status buttons On Off | <u>DISP:WIND:ANN:TRAC:STAT</u> | None                               |
| Memory Trace On Off         | <u>DISP:WIND:TRAC:MEM</u>      | <u>meas.View</u>                   |
| Title Annotation On Off     | <u>DISP:WIND:TITL</u>          | <u>win.TitleState</u>              |
| Error Messages On Off       | <u>DISP:ANN:MESS:STAT</u>      | <u>app.DisplayAutomationErrors</u> |

**Miscellaneous**

|                                                                                                                           |                                |                               |
|---------------------------------------------------------------------------------------------------------------------------|--------------------------------|-------------------------------|
| Make a Title Annotation                                                                                                   | <u>DISP:WIND:TITL:DATA</u>     | <u>win.Title</u>              |
| One Readout per Trace                                                                                                     | <u>DISP:WIND:ANN:MARK:SING</u> | <u>win.OneReadoutPerTrace</u> |
| Marker Readout Size                                                                                                       | <u>DISP:WIND:ANN:MARK:SIZE</u> | <u>win.MarkerReadoutSize</u>  |
| Add a Window                                                                                                              | <u>DISP:WIND</u>               | <u>wins.Add</u>               |
| Return Window Number(s)                                                                                                   | <u>DISP:CATalog?</u>           | <u>win.WindowNumber</u>       |
| Activate a Window                                                                                                         | None                           | <u>app.ActivateWindow</u>     |
| Arrange Measurement Windows                                                                                               | <u>DISP:ARRange</u>            | <u>app.ArrangeWindows</u>     |
|  Analyzer Window<br>(Max  Min  Normal) | <u>DISPlay:WIND:SIZE</u>       | <u>app.WindowState</u>        |

## Bias Input Connectors

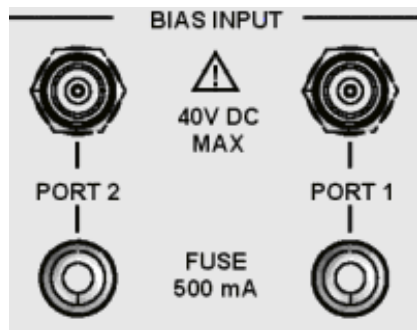

### Test Port Bias Input

Test port bias is standard on E8356A, E8357A, and E8358A models and available as UNL Option on other selected PNA models.

There is NO Test Port Bias on N5230A models.

**Note:** Although connectors and fuses may be present, test port bias may NOT be available.

This BNC(f) connector allows external bias to be applied at the Test Ports.


| PNA Models  | Max Voltage | Fuse rating |
|-------------|-------------|-------------|
| 3, 6, 9 GHz | 30V         | 1A*         |
| Microwave   | 40V         | .5A         |

- \*Up to 200 mA level, the instrument will meet all of its RF specifications. As the DC bias is increased, particularly at low RF frequencies (that is, typically <100 MHz, but predominantly >10 MHz), the low frequency corrected source match and directivity will degrade. Above 100 MHz RF, with up to 1 A bias, there is very little degradation in corrected source match and directivity.

See Rear Panel

## Auxiliary I/O Connector

---

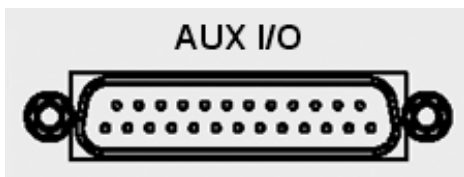

This DB-25 male connector provides a variety of analog I/O, digital I/O, timing I/O, triggering, and supply lines. See details of the [Aux I/O Connector](#).

[See Rear Panel](#)

## External AM Input Connector

---

EXT AM  
INPUT



This BNC(f) connector allows you to input a voltage that provides low-frequency AM modulation to the test port output signal. You could also input a voltage to shift the test port output power level. An input of 0 volts leaves the power level unaffected. A positive voltage input shifts the test port power to a higher level. A negative voltage shifts the power to a lower level.

- Input sensitivity: 8 dB/volt, typical
- Bandwidth: 1 kHz, typical
- Input impedance: 1k  $\Omega$ , typical

---

**Note:** This connector is **ONLY** provided on 3 GHz, 6 GHz, and 9 GHz PNA models.

[See Rear Panel](#)

## External Detector Input Connector

---

### EXT DETECTOR INPUT



This BNC(f) connector allows you to input DC from an external, negative polarity diode detector for controlling the power level at the test ports. To allow the analyzer to accept this external input, you must have the **External ALC** box checked in the Sweep Setup dialog box.

- Input sensitivity:  $-500\text{mV}$  gives approximately  $-3\text{ dBm}$  at the detector input
- Bandwidth: 50 kHz, typical
- Input impedance:  $1\text{ k}\Omega$ , typical

---

**Note:** This connector is **ONLY** provided on 3 GHz, 6 GHz, and 9 GHz PNA models.

---

See Rear Panel

## 10 MHz Reference Connectors

---

10MHz  
INPUT



10MHz  
REF  
OUTPUT



### 10 MHz Reference Input

This BNC(f) connector allows the analyzer to work with an external reference signal.

If a 10 MHz external reference signal is detected at this port, it will be used as the instrument frequency reference instead of the internal frequency reference.

The 10 MHz REF INPUT port has the following characteristics:

- Input frequency: 10 MHz
- Input level:  $-15$  to  $+20$  dBm, typical
- Input impedance:  $200\ \Omega$ , nominal

### 10 MHz Reference Output

This BNC(f) connector provides a frequency reference signal with the following characteristics:

- Output frequency:
  - 10 MHz  $\pm 1$ ppm (PNA models E8356/7/8A and E8362/3/4A)
  - 10 MHz  $\pm 10$ ppm (PNA models E8801/2/3A and N3381/2/3A)  
To upgrade, order [Option 1E5](#).
- Signal type: sine wave
- Output level: 10 dBm  $\pm 4$  dB into 50 ohms
- Output impedance: 50 ohms
- Harmonics:  $< -40$  dBc

[See Rear Panel](#)

## General Purpose Interface Bus (GPIB) Connector

---



This 24-pin connector is a female Type D-24 which is compatible with IEEE-488. It is used to send and receive GPIB / SCPI commands.

[Learn more about GPIB.](#)

[See Rear Panel](#)




## Material Handler I/O Connector

---

A rectangular 36-pin female connector provides the following:

- four independent parallel data ports
- nine control signal lines
- one ground
- one power supply line

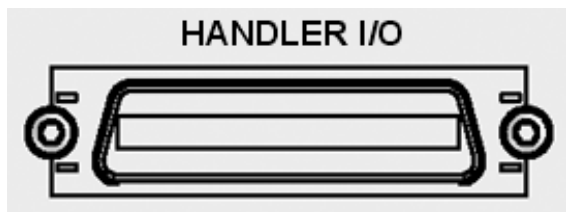

All signals are TTL-compatible.

---

**Note:** On early PNAs this connector is labeled "GPIO". It is covered to indicate that the connector is not functional.


---

See details of the [Material Handler Connector](#)

[See Rear Panel](#)

## Hard Drive

---

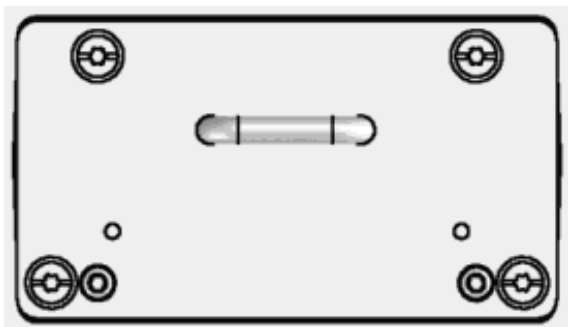

The hard drive on PNA models E836x A/B can be easily removed from this rear panel access. Refer to the PNA Service Guide, chapter 7 for a detailed procedure.

You can download the Service Guide for your PNA model from our website: <http://www.agilent.com>.

[See Rear Panel](#)

## IF Access Connectors

---



Only available with H11 option

### Test Set Drivers

PNA RF Source and LO outputs for external mixing.

### Pulse In

Provides capability to perform pulsed measurements with the H08 option.


### 8.33 MHz IF IN

Provides access to the PNA receiver's IF lines.

See Rear Panel

## Local Area Network (LAN) Connector

---




This 10/100BaseT Ethernet connection has a standard 8-pin configuration and auto selects between the two data rates.

[See Rear Panel](#)

## Parallel Interface Port (LPT1) Connector

---



This DB25 female connector provides connection to a printer or any other parallel port peripheral.

---

**Note:** Early PNA models were shipped with a Centronics connector for connecting a printer. An adapter (36-pin male - 1284-C - to 25-pin female) was shipped with those PNAs to allow connection with a standard parallel printer cable.

---

[See Rear Panel](#)

## Serial Interface Port (COM1) Connector

---




This 9-pin male D-sub connector is RS-232 compatible.

See Rear Panel

## External Test Set I/O Connector

---

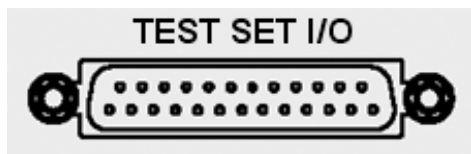

This DB-25 female connector is used to control external test sets. The external test set bus consists of 13 multiplexed address and data lines, three control lines, and an open-collector interrupt line. The bus may be "daisy-chained" from one test set to the next in order to control up to 16 test sets at one time.

---

**Note:** The Test Set I/O is not compatible with Agilent 8753 test sets.

See details of the [External Test Set Connector](#)

[See Rear Panel](#)

## Trigger IN / OUT

---

I/O (TRIG IN)



I/O (TRIG OUT)



These connectors provide triggering capability to and from the PNA. They are available on PNA models E8361A, E836xB, and N5230A. For more information see [External Triggering](#).

[See Rear Panel](#)



## Universal Serial Bus (USB) Connector

---




This Type A Universal Serial Bus (USB) connector allows you to connect a keyboard, mouse, ECAL module, or other USB device.

- Contact 1: Vcc; 4.75 to 5.25 VDC, 500 mA maximum. Protected with an automatically-resettable 1A fuse.
- Contact 2: -Data
- Contact 3: +Data
- Contact 4: Ground

[See USB Limitations](#)

## Universal Serial Bus (USB) Hub

---

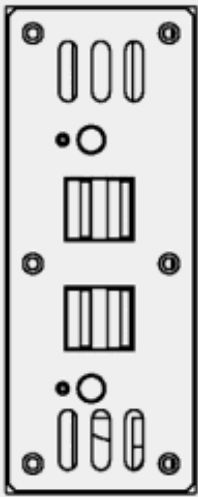

This USB hub contains four USB ports to power your PNA peripherals.

---

**Limitation:** The total power consumption for all six USB ports is limited to 1.5 amps. If this limit is exceeded, all USB ports are disabled until a device is removed and power consumption falls below the limit. (When first connected, Agilent ECAL modules 8509x and N4431 draw significantly more current than other modules.)

---

- This internal USB hub is available on PNA models E8361A, E8362B, E8363B, and E8364B.
- It is relocated on PNA model N5230A.

## Video Graphics Adapter (VGA) Output Connector

---



This 15-pin female D-sub connector allows connection of external VGA monitors. With the following resolution settings, you can simultaneously view the PNA display and a remote monitor.

[See Rear Panel](#)

| External Device   | Resolution                            |
|-------------------|---------------------------------------|
| Flat Panel (TFT)  | 1024x768, 800x600, 640x480            |
| Flat Panel (DSTN) | 800x600, 640x480                      |
| CRT Monitor       | 1280x1024, 1024x768, 800x600, 640x480 |

---

**Note:** To view both the analyzer and the external monitor. If the analyzer is set to the default resolution (640 x 480), you can view both. If you change the analyzer resolution through the control panel to a setting other than the default, you can only view the external monitor. To change the resolution: In the **System** menu, point to **Configure**, then click **Control Panel**. Then click on the **Display** icon and the **Settings** tab.

---

## Perform Administrative Tasks

---

[RNA Users and Passwords](#)

[RNA Computer Properties](#)

[Operating System Recovery](#)

[Select a Local Language for the Help System](#)

## Networking and Connecting the PNA

---

### The PNA as a PC

[PNA User Accounts and Passwords](#)

[Connecting the PNA to a PC](#)

[Easy versus Secure Configuration](#)

[Changing Network Client](#)

[Using VNC to Control the PNA User Interface](#)

### GPIB / COM Programming

[Configure for COM/DCOM Programming](#)

[82357A USB to GPIB Interface](#)

[The PNA as GPIB System Controller](#)

### Controlling External Devices

[5091 TestSet Control](#)

[Interface Control Feature](#)

[Handler IO Connector](#)

[AuxIO Connector](#)

[TestSetIO Connector](#)

## Frequency Blanking

**Note:** To learn how to erase memory before moving your PNA out of a secure area, see <http://na.tm.agilent.com/pna/security.html>.

For security reasons, you can prevent frequency information from appearing on the PNA screen and printouts.


When the security level is set to **Low** or **High**, frequency information is blanked from the following:

- Display annotation
- Calibration properties
- All tables
- All toolbars
- All printouts
- GPIB console  
When set to **None** or **Low**, nothing is blanked.  
When set to **High**, the GPIB console is inactive.


When the Security level is set to **Low** or **High**, frequency information is **NOT** blanked from the following:

- The Frequency Converter Application (opt 083) dialog box information or printouts.
- Service Programs.
- Your COM or SCPI programs.

### How to set Frequency Blanking

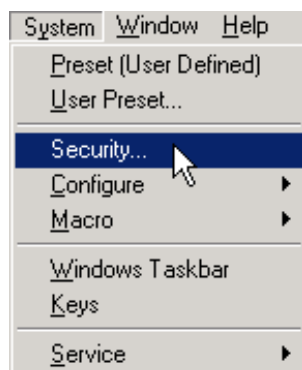

Learn more about using the [front panel interface](#)

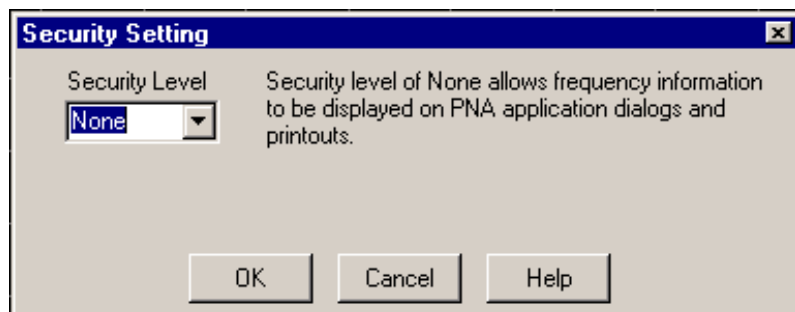

## Security Setting dialog box help

**None** - All frequency information is displayed on the screen and printouts.

**Low** - All frequency information is blanked. However, you can re-display frequency information by revisiting this dialog box and clicking **None**.

**High** - All frequency information is blanked. To re-display frequency information, you must perform an instrument preset, or recall an instrument state with security level of None or Low.

## Quick Start

---

The following topics can help you become familiar with your PNA:

[Front Panel Tour](#)

[Rear Panel Tour](#)

[Powering the PNA ON and OFF](#)

[Front-panel Interface](#)

[Traces, Channels, and Windows](#)

[Basic Measurement Sequence](#)

[Using Help](#)

[Operating System Recovery](#)

[Networking and Connecting the Analyzer](#)

[Perform Administrative Tasks](#)

### VERY IMPORTANT NOTES:

---

1. Do NOT modify or reconfigure the operating system or Agilent's PNA software.
2. The PNA does NOT have antivirus protection. It is strongly recommended that you install antivirus protection if you connect the PNA to the Internet.

For more information see [Windows considerations](#).

---



## Using VNC to Control the PNA User Interface

---

VNC (Virtual Network Computing) allows you to control the User Interface of a PNA from any PC. The PNA display appears on the connected PC display. Mouse and keyboard control can occur from both the PNA and PC, although not simultaneously.

Both the PNA and PC must be connected to the internet. The responsiveness of the PNA while using VNC is dependent of the speed of your internet connection.


Every PNA is shipped with VNC installed. However, you must download and install the VNC software onto the PC from <http://www.realvnc.com/>.

Once installed, the following procedure will help you configure VNC to view and control the PNA application from your PC.

### On the PNA, run VNC Server

To do this:

1. Click View, then Minimize Application.
2. Click **Start, Programs, RealVNC, Run VNC Server.**

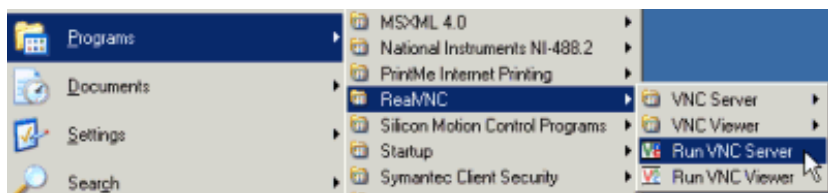

- The first time you run VNC Server, you will set a password to control access from remote PCs.
- To automatically start VNC when the PNA computer boots, drag a **Run VNC Server** shortcut to your User "startup" folder. The following is the Administrator folder: C:\Documents and Settings\Administrator\Start Menu\Programs\Startup

### On the PC, run VNC Viewer

To do this:

1. Download (<http://www.realvnc.com/>) and install VNC on the PC.
2. From the PC Desktop, click **Start, Programs, RealVNC, Run VNC Viewer**
3. When prompted for the Hostname, type the full computer name or IP address of the PNA.
4. When prompted for the password, type the password you set when configuring VNC on the PNA.

## Set Up Measurements

---

You can set up your measurement using the following steps:

[Reset the PNA](#)

[Select a Measurement Parameter](#)

[Set Frequency Range](#)

[Set Power Level](#)

[Set Sweep](#)

[Set Data Format and Scale](#)

[Set Triggering](#)

[Pre-configured Measurement Setups](#)


[Customize the PNA Screen](#)

[Copy Channels](#)

[Connector Care](#)

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

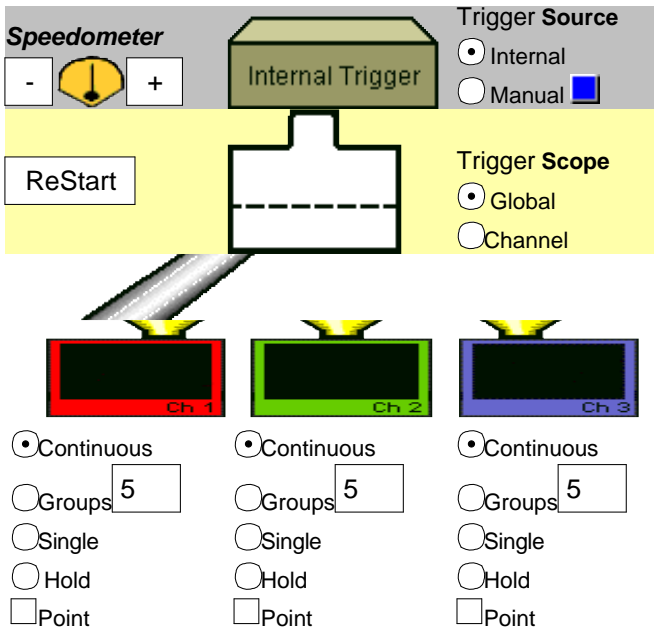

About the trigger model

Read Text description of triggering behaviors.

## Optimize Measurements

---

A measurement has many interdependent settings. You can modify the settings to achieve the goals of your measurement application: faster throughput or greater measurement accuracy.

### Increase Measurement Throughput

[Achieve Fastest Sweep](#)

[Switch Between Multiple Measurements](#)

[Data Transfer Speed](#)

[Using Macros](#)

### Improve Measurement Accuracy

[Increase Dynamic Range](#)

[Increase Number of Data Points](#)

[Improve Phase Measurement Accuracy](#)

[Improve Accuracy for Electrically Long Devices](#)

[Improve Reflection Accuracy on Low-Loss 2-Port Devices](#)

[Increase Measurement Stability](#)

[Reduce Noise](#)

[Decrease Receiver Crosstalk](#)

[Reduce the Effects of Test Accessories](#)

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

---

## Calibrate Measurements

---

[Calibration Overview](#)

[Calibration Wizard](#)

[Select a Calibration](#)

[Using Cal Sets](#)

[Using ECal](#)

[ECal User Characterization](#)

[Error Correction and Interpolation](#)

[Calibration Thru Methods](#)

[Port Extensions](#)

[Fixture Simulator](#)

[Power Calibration](#)

[Accurate Calibrations](#)

[Validity of a Calibration](#)

[Measurement Errors](#)

[Modify Cal Kits](#)

[Calibration Standards](#)

[TRL Cal](#)

To learn how to perform a full 4-port on-wafer calibrations manually using the 4-port 20 GHz PNA-L network analyzer, visit [www.Agilent.com](http://www.Agilent.com) and search for **5989-2287EN**.

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

## Calibration Thru Methods

---

### What is a Non-Insertable Device

#### Choosing a Thru Method

Flush Thru

Adapter Removal

Defined Thru


Unknown Thru

### Other Cal Topics


## What is a Non-Insertable Device

To understand the Thru method choices, you must first understand the following terms. These definitions also apply to ECal modules. Substitute "ECal module" for "device".

A **non-insertable device** is one whose connectors could NOT mate together. They either do not have the same type of connector or they have the same gender. This also means that the test port cables would not mate together, as in the following diagram.

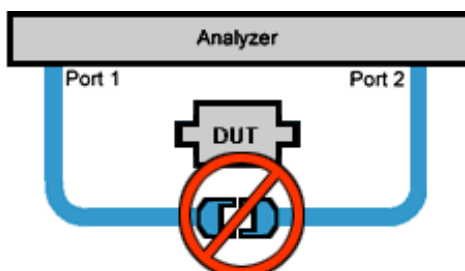

An **insertable device** is one whose connectors could mate together. They have the same type of connector and opposite, or no, gender. This also means that the test port cables would mate together, as in the following diagram.

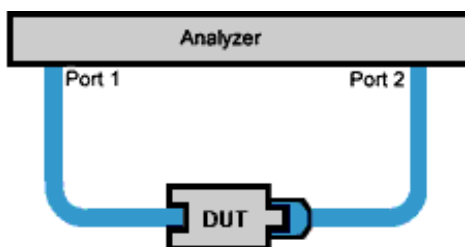

## Choosing a Thru Method of Calibration

The Thru method is selected from the Cal Wizard. Select the **Modify** checkbox in the Select DUT Connectors and

Cal Kits dialog box.

**Notes:**

For ECal, the following choices have different meanings. See [THRU methods for ECal](#).

For 4-port calibration, see [How can we measure only 3 THRU connections?](#)

**Choice for Insertable Devices: FLUSH Thru** (also known as **Zero-length Thru**)

When calibrating for an insertable device, the test ports at your measurement reference plane connect directly together. This is called a zero-length THRU, or Flush THRU meaning that the definition of the THRU standard has zero-length: no delay, no loss, no capacitance, and no inductance. Your calibration kit may not have a THRU standard because it is assumed you have an insertable device and will be using a zero-length THRU.

**Choices for Non-Insertable Devices**

The following methods calibrate for a non-insertable device:

- [Adapter Removal](#) Accurate, but least convenient.
- [Defined Thru](#)
- [Unknown Thru Cal](#) **Preferred method.**
- Swap-Equal-Adapters Method is NOT recommended in the PNA.

**Adapter Removal Calibration**

This method is potentially very accurate. However, it requires many connections which increases the chances of inaccurate data.

Two full 2-port calibrations are performed: one with the adapter connected at port 1, and the other with the adapter connected to port 2. The result of the two calibrations is a single full 2-port calibration that includes accurate characterization and removal of the mismatch caused by the adapter.

Performing an Adapter Removal Cal requires:

- a THRU adapter with connectors that match those on the DUT.
- calibration standards for both DUT connectors.

**Defined Thru** (also known as **Cal Kit Thru**, **ECal Thru**, **Characterized Thru**, **Known Thru**)

---

**Note:** If performing an ECal calibration, this is the THRU standard in the ECal Module.

---

Defined Thru uses the THRU definition that is stored in the Cal Kit file or ECal module. The THRU standard may have worn over time, making it not as accurate as when it was new.

Defined Thru is usually more accurate than Adapter Removal, but not as accurate as Unknown Thru method.

To Define a THRU standard in a Cal Kit (not ECal module):

1. From the PNA Menu, click Calibration, [Advanced Modify Cal Kits](#).
2. Select the Cal Kit
3. Click Edit Kit
4. Click Add

5. Select THRU
6. Complete the dialog box.

The next time you perform a Guided Cal, this Defined THRU standard will be available if the DUT connector types match the THRU standard.

### Unknown Thru Cal

Unknown Thru Cal is the **preferred** method of calibrating the PNA to measure a non-insertable device.

To perform an Unknown Thru, the PNA measures the THRU standard during the calibration process. The resulting data is used to improve the transmission tracking error term.

At the end of the calibration, the PNA estimates the electrical length of the adapter. This estimate may be wrong if there are too few frequency points over the given frequency span. You can compute and change the delay by calculating the physical length of the adapter divided by the propagation velocity:  $\text{Delay} = \text{Length} / \text{Propagation velocity}$

See [Using ECAL](#) for ECAL Thru calibration.

#### Unknown Thru notes:

- Unknown Thru is NOT supported in a TRL calibration.
- Beginning with PNA code release 5.24:
  - The measurement of calibration standards is performed in a dedicated PNA window which becomes visible during the calibration process. Previously, the 16th window was used to perform Unknown Thru standard measurements. This is no longer necessary.
  - Unknown Thru CAN be performed using a PNA that does NOT have a reference receiver for each port. This Cal requires a [Delta Match Calibration](#) be performed before the Unknown Thru is measured.



## Delta Match Calibration

---

Delta Match Calibration makes it possible for you to perform a [TRL Cal](#) or [Unknown Thru Cal](#) on PNA models that do NOT have a reference receiver for each test port. This is the case with the 4-port PNA model. See [PNA configurations](#).

The Delta Match Calibration measures the source match and load match of the PNA test ports, and then calculates the differences, or "delta", of the two match terms. The results are then used to correct subsequent TRL or Unknown Thru calibrations.

The Delta Match Calibration can be acquired in three different ways:

1. During the TRL or Unknown Thru Calibration setup. This is possible if the TRL or Unknown Thru setup is such that all ports to be calibrated are "touched" using a [Defined Thru](#) or [Flush Thru](#). For example, during a 4-port TRL Cal, ports 1 and 2 can be connected using a Flush Thru, and the same is true for ports 3 and 4.
2. From an existing Cal Set that meets the following Delta Match criteria:
  - Must have been performed using ECal or as a guided mechanical Cal (not Unguided).
  - Must have the same start frequency, stop frequency, and number of points as the channel being calibrated.
  - Must calibrate the ports that require the delta match terms. The Cal sets appear in the list.
3. From the [Global Delta Match Calibration](#).


During a [Guided Calibration](#), if a Delta Match Cal is required, the Cal Wizard first tries to use the current calibration setup from which to calculate the delta match terms. If this is not possible, the [Select Delta Match Cal Set](#) dialog is presented allowing you to choose from an existing Cal Set or the Global Delta Match Cal Set.

### Global Delta Match Cal

A Global Delta Match Cal is an "all-inclusive" calibration that can be applied whenever the delta match terms are required. A Global Delta Match Cal differs from a standard SOLT Cal in the following ways:

- It is always performed using a Flush Thru, a Known Thru, or an insertable ECal module. You can NOT use an Unknown Thru in the calibration process.
- Only two Thru connections are required to characterize the delta match terms on a 4-port PNA. This is less than the minimum number of Thrus of a standard 4-port Cal.
- Upon completion, the Global Delta Match Cal is stored as a special type of Cal Set and should be used ONLY as a Delta Match Cal. It provides Delta Match error terms, but does NOT provide all of the standard error correction terms.
- To attain the highest accuracy, the following settings are automatically used to perform a Global Delta Match Cal. When applied, it will likely be [interpolated](#), but without compromising quality.
  - Performed over the entire frequency range of the PNA.
  - Uses 1601 measurement points.
  - Uses 100 Hz IF Bandwidth.

## How to perform a Global Delta Match Cal

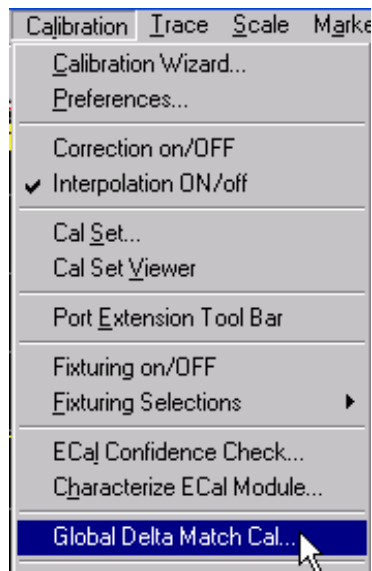

Learn more about using the [front panel interface](#)



### Delta Match Calibration. Select DUT Connectors and Cal Kit dialog box help


- Only one Cal Kit is specified and necessary to perform a Delta Match Cal. However, ALL of the PNA test ports are calibrated in a Delta Match Cal.
- You must configure ALL test ports to terminate in the specified connector / gender using the necessary adapters. The errors from adapters are removed during calibration, but the Thru connections must be made as specified.
- **If you select an ECal module that does NOT cover the entire frequency range of the PNA, your selection will change to a different Cal Kit. The Global Delta Match Cal covers the entire frequency range of the PNA. Your selected Cal Kit or ECal module must also cover the frequency range of the PNA.**



### Guided Calibration Steps dialog box help

Click **Measure** for each standard.

When all standards have been measured, click **Done** to complete the measurement steps.

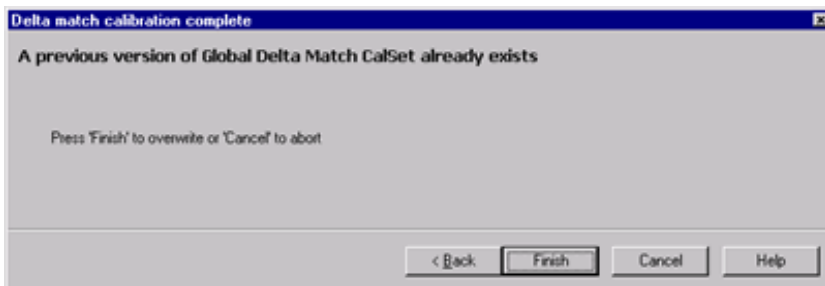

### Delta Match Calibration Complete dialog box help

Click **Finish** to store the Global Delta Match Calibration as a special type of Cal Set. It is offered as a choice when a Delta Match Calibration is required.

It should ONLY be used as a Delta Match Cal. It does NOT provide all of the standard error correction terms.

## Analyze Data

---

[Locate Data Using Markers](#)

[Manipulate Data Using Math Operations](#)

[Using Limit Lines to Test Devices](#)

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

## Print, Save, and Recall Data

---

[Save and Recall a File](#)

[Print a Displayed Measurement](#)

[Drive Mapping](#)


---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

## Specifications: Front-Panel Jumpers

### Models E8362A/B, E8363A/B, and E8364A/B Option 014

**NOTE:** The standard E8362/3/4A/B has no front-panel jumpers.

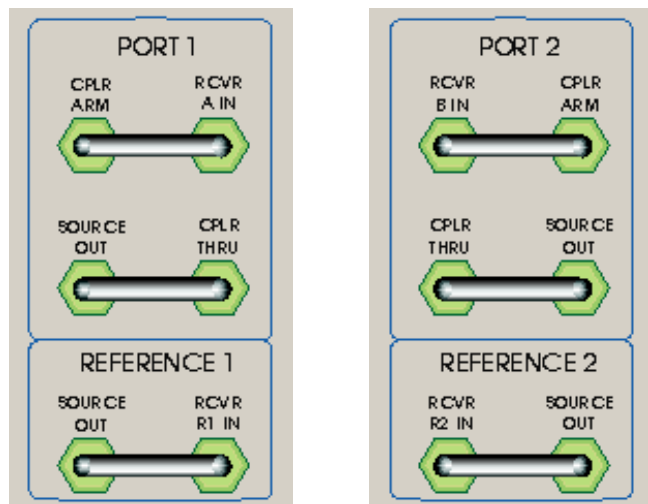

**Measurement Receiver Inputs (Rcvr A In, Rcvr B In)**

**Reference Receiver Inputs (Rcvr R1 In, Rcvr R2 In)**

**Reference Outputs (Reference 1 Source Out, Reference 2 Source Out)**

**Source Outputs (Port 1 Source Out, Port 2 Source Out)**

**Coupler Inputs (Port 1 Coupler Thru, Port 2 Coupler Thru)**

**Coupler Outputs (Port 1 Coupler Arm, Port 2 Coupler Arm)**

**Table 47: Measurement Receiver Inputs (Rcvr A In, Rcvr B In)**

| Description                | Specification | Supplemental Information |
|----------------------------|---------------|--------------------------|
| <b>Maximum Input Level</b> |               |                          |
| <b>E8362A/B:</b>           |               |                          |
| 45 MHz to 500 MHz          |               | -15 dBm, typical         |
| 500 MHz to 2 GHz           |               | -11 dBm, typical         |
| 2 GHz to 10 GHz            |               | -11 dBm, typical         |
| 10 GHz to 20 GHz           |               | -11 dBm, typical         |
| <b>E8363A/B:</b>           |               |                          |
| 45 MHz to 500 MHz          |               | -14 dBm, typical         |

|                    |                           |                     |
|--------------------|---------------------------|---------------------|
| 500 MHz to 2 GHz   |                           | -10 dBm, typical    |
| 2 GHz to 10 GHz    |                           | -10 dBm, typical    |
| 10 GHz to 20 GHz   |                           | -10 dBm, typical    |
| 20 GHz to 30 GHz   |                           | -14.5 dBm, typical  |
| 30 GHz to 40 GHz   |                           | -16.5 dBm, typical  |
| <b>E8364A/B:</b>   |                           |                     |
| 45 MHz to 500 MHz  |                           | - 14 dBm, typical   |
| 500 MHz to 2 GHz   |                           | - 10 dBm, typical   |
| 2 GHz to 10 GHz    |                           | - 10 dBm, typical   |
| 10 GHz to 20 GHz   |                           | - 10 dBm, typical   |
| 20 GHz to 30 GHz   |                           | - 14.5 dBm, typical |
| 30 GHz to 40 GHz   |                           | - 16.5 dBm, typical |
| 40 GHz to 45 GHz   |                           | - 16 dBm, typical   |
| 45 GHz to 50 GHz   |                           | - 15 dBm, typical   |
| <b>Noise Floor</b> |                           |                     |
| <b>E8362A/B:</b>   |                           |                     |
|                    | <b>10 Hz IF Bandwidth</b> |                     |
| 45 MHz to 500 MHz  | < -109 dBm                |                     |
| 500 MHz to 2 GHz   | < -130 dBm                |                     |
| 2 GHz to 10 GHz    | < -133 dBm                |                     |
| 10 GHz to 20 GHz   | < -135 dBm                |                     |
|                    | <b>1 kHz IF Bandwidth</b> |                     |
| 45 MHz to 500 MHz  | < -89 dBm                 |                     |
| 500 MHz to 2 GHz   | < -110 dBm                |                     |
| 2 GHz to 10 GHz    | < -113 dBm                |                     |
| 10 GHz to 20 GHz   | < -115 dBm                |                     |
| <b>E8363A/B:</b>   |                           |                     |

|                   |                           |  |
|-------------------|---------------------------|--|
|                   | <b>10 Hz IF Bandwidth</b> |  |
| 45 MHz to 500 MHz | < -127 dBm                |  |
| 500 MHz to 2 GHz  | < -133 dBm                |  |
| 2 GHz to 10 GHz   | < -132 dBm                |  |
| 10 GHz to 20 GHz  | < -134 dBm                |  |
| 20 GHz to 40 GHz  | < -125 dBm                |  |
|                   | <b>1 kHz IF Bandwidth</b> |  |
| 45 MHz to 500 MHz | < -107 dBm                |  |
| 500 MHz to 2 GHz  | < -113 dBm                |  |
| 2 GHz to 10 GHz   | < -112 dBm                |  |
| 10 GHz to 20 GHz  | < -114 dBm                |  |
| 20 GHz to 40 GHz  | < -105 dBm                |  |
| <b>E8364A/B:</b>  |                           |  |
|                   | <b>10 Hz IF Bandwidth</b> |  |
| 45 MHz to 500 MHz | < - 127 dBm               |  |
| 500 MHz to 2 GHz  | < - 133 dBm               |  |
| 2 GHz to 10 GHz   | < - 132 dBm               |  |
| 10 GHz to 20 GHz  | < - 134 dBm               |  |
| 20 GHz to 40 GHz  | < - 125 dBm               |  |
| 40 GHz to 50 GHz  | < - 123 dBm               |  |
|                   | <b>1 kHz IF Bandwidth</b> |  |
| 45 MHz to 500 MHz | < -107 dBm                |  |
| 500 MHz to 2 GHz  | < -113 dBm                |  |
| 2 GHz to 10 GHz   | < -112 dBm                |  |
| 10 GHz to 20 GHz  | < -114 dBm                |  |
| 20 GHz to 40 GHz  | < -105 dBm                |  |
| 40 GHz to 50 GHz  | < -103 dBm                |  |



| Damage Level     |  |                   |
|------------------|--|-------------------|
| E8362A/B         |  | + 15 dBm, typical |
| E8363A/B         |  | + 15 dBm, typical |
| E8364A/B         |  | + 15 dBm, typical |
| Maximum DC Level |  |                   |
| E8362A/B         |  | + 15 V, typical   |
| E8363A/B         |  | + 15 V, typical   |
| E8364A/B         |  | + 15 V, typical   |

**Table 48: Reference Receiver Inputs (Rcvr R1, Rcvr R2)**

| Description         | Specification | Supplemental Information |
|---------------------|---------------|--------------------------|
| Maximum Input Level |               |                          |
| <b>E8362A/B:</b>    |               |                          |
| 45 MHz to 500 MHz   |               | -15 dBm, typical         |
| 500 MHz to 2 GHz    |               | -11 dBm, typical         |
| 2 GHz to 10 GHz     |               | -11 dBm, typical         |
| 10 GHz to 20 GHz    |               | -11 dBm, typical         |
| <b>E8363A/B:</b>    |               |                          |
| 45 MHz to 500 MHz   |               | -14 dBm, typical         |
| 500 MHz to 2 GHz    |               | -10 dBm, typical         |
| 2 GHz to 10 GHz     |               | -10 dBm, typical         |
| 10 GHz to 20 GHz    |               | -9.5 dBm, typical        |
| 20 GHz to 30 GHz    |               | -14 dBm, typical         |
| 30 GHz to 40 GHz    |               | -15.5 dBm, typical       |
| <b>E8364A/B:</b>    |               |                          |
| 45 MHz to 500 MHz   |               | - 14 dBm, typical        |
| 500 MHz to 2 GHz    |               | - 10 dBm, typical        |
| 2 GHz to 10 GHz     |               | - 10 dBm, typical        |

|                         |  |                     |
|-------------------------|--|---------------------|
| 10 GHz to 20 GHz        |  | - 9.5 dBm, typical  |
| 20 GHz to 30 GHz        |  | - 14 dBm, typical   |
| 30 GHz to 40 GHz        |  | - 15.5 dBm, typical |
| 40 GHz to 45 GHz        |  | - 14 dBm, typical   |
| 45 GHz to 50 GHz        |  | - 15 dBm, typical   |
| <b>Damage Level</b>     |  |                     |
| E8362A/B                |  | + 15 dBm, typical   |
| E8363A/B                |  | + 15 dBm, typical   |
| E8364A/B                |  | + 15 dBm, typical   |
| <b>Maximum DC Level</b> |  |                     |
| E8362A/B                |  | +/- 15 V, typical   |
| E8363A/B                |  | +/- 15 V, typical   |
| E8364A/B                |  | +/- 15 V, typical   |

**Table 49: Reference Outputs (Reference 1 Source Out, Reference 2 Source Out)**

| Description                 | Specification | Supplemental Information |
|-----------------------------|---------------|--------------------------|
| <b>Maximum Output Level</b> |               |                          |
| <b>E8362A/B:</b>            |               |                          |
| 45 MHz to 500 MHz           |               | -24 dBm, typical         |
| 500 MHz to 2 GHz            |               | -23 dBm, typical         |
| 2 GHz to 10 GHz             |               | -23 dBm, typical         |
| 10 GHz to 20 GHz            |               | -26 dBm, typical         |
| <b>E8363A/B:</b>            |               |                          |
| 45 MHz to 500 MHz           |               | -11.5 dBm, typical       |
| 500 MHz to 2 GHz            |               | -10.5 dBm, typical       |
| 2 GHz to 10 GHz             |               | -11 dBm, typical         |
| 10 GHz to 20 GHz            |               | -11 dBm, typical         |
| 20 GHz to 30 GHz            |               | -11 dBm, typical         |

|                         |  |                     |
|-------------------------|--|---------------------|
| 30 GHz to 40 GHz        |  | -11 dBm, typical    |
| <b>E8364A/B:</b>        |  |                     |
| 45 MHz to 500 MHz       |  | - 11.5 dBm, typical |
| 500 MHz to 2 GHz        |  | - 10.5 dBm, typical |
| 2 GHz to 10 GHz         |  | - 11 dBm, typical   |
| 10 GHz to 20 GHz        |  | - 11 dBm, typical   |
| 20 GHz to 30 GHz        |  | - 11 dBm, typical   |
| 30 GHz to 40 GHz        |  | - 11 dBm, typical   |
| 40 GHz to 45 GHz        |  | - 11 dBm, typical   |
| 45 GHz to 50 GHz        |  | - 15 dBm, typical   |
| <b>Damage Level</b>     |  |                     |
| E8362A/B                |  | + 20 dBm, typical   |
| E8363A/B                |  | + 20 dBm, typical   |
| E8364A/B                |  | + 20 dBm, typical   |
| <b>Maximum DC Level</b> |  |                     |
| E8362A/B                |  | +/- 15 V, typical   |
| E8363A/B                |  | +/- 15 V, typical   |
| E8364A/B                |  | +/- 15 V, typical   |

**Table 50: Source Outputs (Port 1 Source Out, Port 2 Source Out)**

| Description                  | Specification | Supplemental Information |
|------------------------------|---------------|--------------------------|
| <b>Maximum Output Level</b>  |               |                          |
| <b>E8362A/B, Option 014:</b> |               |                          |
| 45 MHz to 500 MHz            |               | 6 dBm, typical           |
| 500 MHz to 2 GHz             |               | 7 dBm, typical           |
| 2 GHz to 10 GHz              |               | 7 dBm, typical           |
| 10 GHz to 20 GHz             |               | 4 dBm, typical           |

| <b>E8362A/B, Option 014 and UNL:</b> |  |                   |
|--------------------------------------|--|-------------------|
| 45 MHz to 500 MHz                    |  | 4 dBm, typical    |
| 500 MHz to 2 GHz                     |  | 5 dBm, typical    |
| 2 GHz to 10 GHz                      |  | 5 dBm, typical    |
| 10 GHz to 20 GHz                     |  | 2 dBm, typical    |
| <b>E8363A/B, Option 014:</b>         |  |                   |
| 45 MHz to 500 MHz                    |  | 5.5 dBm, typical  |
| 500 MHz to 2 GHz                     |  | 6.5 dBm, typical  |
| 2 GHz to 10 GHz                      |  | 6.5 dBm, typical  |
| 10 GHz to 20 GHz                     |  | 4 dBm, typical    |
| 20 GHz to 30 GHz                     |  | 10 dBm, typical   |
| 30 GHz to 40 GHz                     |  | -2 dBm, typical   |
| <b>E8363A/B, Option 014 and UNL:</b> |  |                   |
| 45 MHz to 500 MHz                    |  | 3.5 dBm, typical  |
| 500 MHz to 2 GHz                     |  | 5 dBm, typical    |
| 2 GHz to 10 GHz                      |  | 5 dBm, typical    |
| 10 GHz to 20 GHz                     |  | 3.5 dBm, typical  |
| 20 GHz to 30 GHz                     |  | 0 dBm, typical    |
| 30 GHz to 40 GHz                     |  | -2.5 dBm, typical |
| <b>E8364A/B, Option 014:</b>         |  |                   |
| 45 MHz to 500 MHz                    |  | 5.5 dBm, 0typical |
| 500 MHz to 2 GHz                     |  | 6.5 dBm, typical  |
| 2 GHz to 10 GHz                      |  | 6.5 dBm, typical  |
| 10 GHz to 20 GHz                     |  | 4 dBm, typical    |
| 20 GHz to 30 GHz                     |  | 1 dBm, typical    |
| 30 GHz to 40 GHz                     |  | -2 dBm, typical   |
| 40 GHz to 45 GHz                     |  | -3 dBm, typical   |

|                                      |  |                   |
|--------------------------------------|--|-------------------|
| 45 GHz to 50 GHz                     |  | -7.5 dBm, typical |
| <b>E8364A/B, Option 014 and UNL:</b> |  |                   |
| 45 MHz to 500 MHz                    |  | 3.5 dBm, typical  |
| 500 MHz to 2 GHz                     |  | 5 dBm, typical    |
| 2 GHz to 10 GHz                      |  | 5 dBm, typical    |
| 10 GHz to 20 GHz                     |  | 3.5 dBm, typical  |
| 20 GHz to 30 GHz                     |  | 0 dBm, typical    |
| 30 GHz to 40 GHz                     |  | -2.5 dBm, typical |
| 40 GHz to 45 GHz                     |  | -5 dBm, typical   |
| 45 GHz to 50 GHz                     |  | -10 dBm, typical  |
| <b>Damage Level</b>                  |  |                   |
| E8362A/B                             |  | 20 dBm, typical   |
| E8363A/B                             |  | 20 dBm, typical   |
| E8364A/B                             |  | 20 dBm, typical   |
| <b>Maximum DC Level</b>              |  |                   |
| E8362A/B                             |  | 0 V, typical      |
| E8363A/B                             |  | 0 V, typical      |
| E8364A/B                             |  | 0 V, typical      |

**Table 51: Coupler Inputs (Port 1 Cplr Thru, Port 2 Cplr Thru)**

| Description                        | Specification | Supplemental Information |
|------------------------------------|---------------|--------------------------|
| <b>Insertion Loss to Test Port</b> |               |                          |
| <b>E8362A/B, Option 014:</b>       |               |                          |
| 45 MHz to 500 MHz                  |               | 0.5 dB, typical          |
| 500 MHz to 2 GHz                   |               | 1.5 dB, typical          |
| 2 GHz to 10 GHz                    |               | 1.5 dB, typical          |
| 10 GHz to 20 GHz                   |               | 1.5 dB, typical          |

| <b>E8362A/B, Option 014 and UNL:</b> |  |                 |
|--------------------------------------|--|-----------------|
| 45 MHz to 500 MHz                    |  | 1 dB, typical   |
| 500 MHz to 2 GHz                     |  | 2 dB, typical   |
| 2 GHz to 10 GHz                      |  | 2 dB, typical   |
| 10 GHz to 20 GHz                     |  | 2 dB, typical   |
| <b>E8363A/B, Option 014:</b>         |  |                 |
| 45 MHz to 500 MHz                    |  | 0.5 dB, typical |
| 500 MHz to 2 GHz                     |  | 0.5 dB, typical |
| 2 GHz to 10 GHz                      |  | 1.5 dB, typical |
| 10 GHz to 20 GHz                     |  | 2 dB, typical   |
| 20 GHz to 30 GHz                     |  | 3 dB, typical   |
| 30 GHz to 40 GHz                     |  | 3.5 dB, typical |
| <b>E8363A/B, Option 014 and UNL:</b> |  |                 |
| 45 MHz to 500 MHz                    |  | 0.5 dB, typical |
| 500 MHz to 2 GHz                     |  | 1 dB, typical   |
| 2 GHz to 10 GHz                      |  | 2 dB, typical   |
| 10 GHz to 20 GHz                     |  | 3 dB, typical   |
| 20 GHz to 30 GHz                     |  | 4 dB, typical   |
| 30 GHz to 40 GHz                     |  | 5 dB, typical   |
| <b>E8364A/B, Option 014:</b>         |  |                 |
| 45 MHz to 500 MHz                    |  | 0.5 dB, typical |
| 500 MHz to 2 GHz                     |  | 0.5 dB, typical |
| 2 GHz to 10 GHz                      |  | 1.5 dB, typical |
| 10 GHz to 20 GHz                     |  | 2 dB, typical   |
| 20 GHz to 30 GHz                     |  | 3 dB, typical   |
| 30 GHz to 40 GHz                     |  | 3.5 dB, typical |
| 40 GHz to 45 GHz                     |  | 3.5 dB, typical |

|                                      |  |                   |
|--------------------------------------|--|-------------------|
| 45 GHz to 50 GHz                     |  | 4 dB, typical     |
| <b>E8364A/B, Option 014 and UNL:</b> |  |                   |
| 45 MHz to 500 MHz                    |  | 0.5 dB, typical   |
| 500 MHz to 2 GHz                     |  | 1 dB, typical     |
| 2 GHz to 10 GHz                      |  | 2 dB, typical     |
| 10 GHz to 20 GHz                     |  | 3 dB, typical     |
| 20 GHz to 30 GHz                     |  | 4 dB, typical     |
| 30 GHz to 40 GHz                     |  | 5 dB, typical     |
| 40 GHz to 45 GHz                     |  | 5.5 dB, typical   |
| 45 GHz to 50 GHz                     |  | 6 dB, typical     |
| <b>Damage Level</b>                  |  |                   |
| E8362A/B                             |  | + 30 dBm, typical |
| E8363A/B                             |  | + 30 dBm, typical |
| E8364A/B                             |  | + 30 dBm, typical |
| <b>Maximum DC Level</b>              |  |                   |
| E8362A/B                             |  | +/- 40 V, typical |
| E8363A/B                             |  | +/- 40 V, typical |
| E8364A/B                             |  | +/- 40 V, typical |

**Table 52: Coupler Outputs (Port 1 Cplr Arm, Port 2 Cplr Arm)**


| Description             | Specification | Supplemental Information |
|-------------------------|---------------|--------------------------|
| <b>Damage Level</b>     |               |                          |
| E8362A/B                |               | + 30 dBm, typical        |
| E8363A/B                |               | + 30 dBm, typical        |
| E8364A/B                |               | + 30 dBm, typical        |
| <b>Maximum DC Level</b> |               |                          |
| E8362A/B                |               | +/- 7 V, typical         |
| E8363A/B                |               | +/- 7 V, typical         |
| E8364A/B                |               | +/- 7 V, typical         |



## Specifications: Front-Panel Jumpers

### Model E8361A Option 014

**NOTE:** The standard E8361A has no front-panel jumpers.

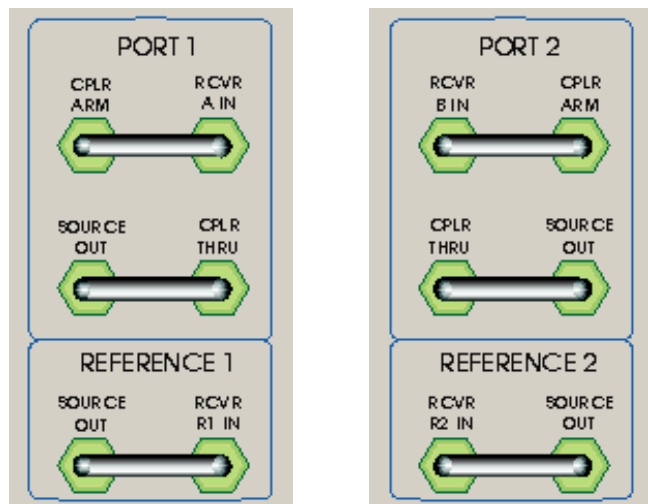

**Measurement Receiver Inputs (Rcvr A In, Rcvr B In)**

**Reference Receiver Inputs (Rcvr R1 In, Rcvr R2 In)**

**Reference Outputs (Reference 1 Source Out, Reference 2 Source Out)**

**Source Outputs (Port 1 Source Out, Port 2 Source Out)**

**Coupler Inputs (Port 1 Coupler Thru, Port 2 Coupler Thru)**

**Coupler Outputs (Port 1 Coupler Arm, Port 2 Coupler Arm)**

**Table 23:** Measurement Receiver Inputs (Rcvr A In, Rcvr B In)

| Description                | Specification | Supplemental Information |
|----------------------------|---------------|--------------------------|
| <b>Maximum Input Level</b> |               |                          |
| <b>E8361A:</b>             |               |                          |
|                            |               | <b>typical:</b>          |
| 10 MHz to 45 MHz           |               | - 12 dBm                 |
| 45 MHz to 500 MHz          |               | - 12 dBm                 |
| 500 MHz to 2 GHz           |               | - 10 dBm                 |
| 2 GHz to 5 GHz             |               | - 10 dBm                 |
| 5 GHz to 10 GHz            |               | - 7 dBm                  |

|                         |  |          |
|-------------------------|--|----------|
| 10 GHz to 24 GHz        |  | - 7 dBm  |
| 24 GHz to 30 GHz        |  | - 7 dBm  |
| 30 GHz to 40 GHz        |  | - 8 dBm  |
| 40 GHz to 45 GHz        |  | - 8 dBm  |
| 45 GHz to 50 GHz        |  | - 8 dBm  |
| 50 GHz to 60 GHz        |  | - 8 dBm  |
| 60 GHz to 67 GHz        |  | - 8 dBm  |
| 67 GHz to 70 GHz        |  | - 8 dBm  |
| <b>Damage Level</b>     |  |          |
| E8361A                  |  | + 15 dBm |
| <b>Maximum DC Level</b> |  |          |
| E8361A                  |  | + 15 V   |

**Table 24:** Reference Receiver Inputs (Rcvr R1, Rcvr R2)

| Description                | Specification | Supplemental Information |                                |
|----------------------------|---------------|--------------------------|--------------------------------|
| <b>Maximum Input Level</b> |               |                          |                                |
| <b>E8361A:</b>             |               |                          |                                |
|                            |               |                          | <b>Rcvr R1 with Option 081</b> |
|                            |               | <b>typical:</b>          |                                |
| 10 MHz to 45 MHz           |               | - 10 dBm                 | - 5.5 dBm                      |
| 45 MHz to 500 MHz          |               | - 9.5 dBm                | - 5.0 dBm                      |
| 500 MHz to 2 GHz           |               | - 9 dBm                  | - 4.0 dBm                      |
| 2 GHz to 5 GHz             |               | - 7.5 dBm                | - 2.0 dBm                      |
| 5 GHz to 10 GHz            |               | - 2.5 dBm                | 3.0 dBm                        |
| 10 GHz to 24 GHz           |               | - 1.5 dBm                | 4.5 dBm                        |
| 24 GHz to 30 GHz           |               | - 0.50 dBm               | 5.5 dBm                        |
| 30 GHz to 40 GHz           |               | - 1 dBm                  | 5.5 dBm                        |
| 40 GHz to 45 GHz           |               | - 0.5 dBm                | 6.5 dBm                        |

|                         |  |          |           |
|-------------------------|--|----------|-----------|
| 45 GHz to 50 GHz        |  | 0 dBm    | 7.0 dBm   |
| 50 GHz to 60 GHz        |  | 0.5 dBm  | 7.50 dBm  |
| 60 GHz to 67 GHz        |  | 1.00 dBm | 9.00 dBm  |
| 67 GHz to 70 GHz        |  | 1.50 dBm | 10.50 dBm |
| <b>Damage Level</b>     |  |          |           |
| E8361A                  |  | + 15 dBm |           |
| <b>Maximum DC Level</b> |  |          |           |
| E8361A                  |  | +/- 15 V |           |

**Table 25:** Reference Outputs (Reference 1 Source Out, Reference 2 Source Out)

| Description                 | Specification | Supplemental Information |                                |                           |
|-----------------------------|---------------|--------------------------|--------------------------------|---------------------------|
| <b>Maximum Output Level</b> |               |                          |                                |                           |
| <b>E8361A:</b>              |               |                          |                                |                           |
|                             |               |                          | <b>Option 014 &amp; UNL</b>    |                           |
|                             |               |                          | <b>Rcvr R1 with Option 081</b> | <b>Without Option 081</b> |
|                             |               | <b>typical:</b>          |                                |                           |
| 10 MHz to 45 MHz            |               | - 43 dBm                 | - 38.5 dBm                     | - 43 dBm                  |
| 45 MHz to 500 MHz           |               | - 17.5 dBm               | - 13 dBm                       | - 17.5 dBm                |
| 500 MHz to 2 GHz            |               | - 12.5 dBm               | - 8.5 dBm                      | - 13.5 dBm                |
| 2 GHz to 5 GHz              |               | - 10.5 dBm               | - 6 dBm                        | - 11.5 dBm                |
| 5 GHz to 10 GHz             |               | - 10.5 dBm               | - 6 dBm                        | - 11.5 dBm                |
| 10 GHz to 24 GHz            |               | - 9.5 dBm                | - 6.5 dBm                      | - 12.5 dBm                |
| 24 GHz to 30 GHz            |               | - 9 dBm                  | - 6 dBm                        | - 12.0 dBm                |
| 30 GHz to 40 GHz            |               | - 9.5 dBm                | - 6 dBm                        | - 12.5 dBm                |

|                         |  |            |           |            |
|-------------------------|--|------------|-----------|------------|
| 40 GHz to 45 GHz        |  | - 13 dBm   | - 10 dBm  | - 17 dBm   |
| 45 GHz to 50 GHz        |  | - 8.5 dBm  | - 5.5 dBm | - 12.5 dBm |
| 50 GHz to 60 GHz        |  | - 9 dBm    | - 6 dBm   | - 13 dBm   |
| 60 GHz to 67 GHz        |  | - 10.5 dBm | - 8.5 dBm | - 16.5 dBm |
| 67 GHz to 70 GHz        |  | - 9 dBm    | - 6 dBm   | - 15 dBm   |
| <b>Damage Level</b>     |  |            |           |            |
| E8361A                  |  | + 20 dBm   |           |            |
| <b>Maximum DC Level</b> |  |            |           |            |
| E8361A                  |  | +/- 15 V   |           |            |

**Table 26:** Source Outputs (Port 1 Source Out, Port 2 Source Out)

| Description                 | Specification |                 | Supplemental Information    |
|-----------------------------|---------------|-----------------|-----------------------------|
| <b>Maximum Output Level</b> |               |                 |                             |
| <b>E8361A</b>               |               |                 |                             |
|                             |               |                 | <b>Option 014 &amp; UNL</b> |
|                             |               | <b>typical:</b> |                             |
| 10 MHz to 45 MHz            |               | -6.5 dBm        | - 5 dBm                     |
| 45 MHz to 500 MHz           |               | -2.5 dBm        | - 1 dBm                     |
| 500 MHz to 2 GHz            |               | -1 dBm          | 1.5 dBm                     |
| 2 GHz to 5 GHz              |               | -1.5 dBm        | 2.5 dBm                     |
| 5 GHz to 10 GHz             |               | -1.5 dBm        | 2.5 dBm                     |
| 10 GHz to 24 GHz            |               | -2 dBm          | 2 dBm                       |
| 24 GHz to 30 GHz            |               | -3 dBm          | 3 dBm                       |
| 30 GHz to 40 GHz            |               | -1 dBm          | 1.5 dBm                     |
| 40 GHz to 45 GHz            |               | -2.5 dBm        | - 3.5 dBm                   |

|                         |  |          |           |
|-------------------------|--|----------|-----------|
| 45 GHz to 50 GHz        |  | -2 dBm   | 1 dBm     |
| 50 GHz to 60 GHz        |  | 0 dBm    | - 0.5 dBm |
| 60 GHz to 67 GHz        |  | -2 dBm   | - 4.5 dBm |
| 67 GHz to 70 GHz        |  | -0.5 dBm | - 1 dBm   |
| <b>Damage Level</b>     |  |          |           |
| E8361A                  |  | 27 dBm   |           |
| <b>Maximum DC Level</b> |  |          |           |
| E8361A                  |  | +/- 40 V |           |

**Table 27:** Coupler Inputs (Port 1 Cplr Thru, Port 2 Cplr Thru)

| Description                        | Specification |                 | Supplemental Information    |
|------------------------------------|---------------|-----------------|-----------------------------|
| <b>Insertion Loss to Test Port</b> |               |                 |                             |
| <b>E8361A</b>                      |               |                 |                             |
|                                    |               |                 | <b>Option 014 &amp; UNL</b> |
|                                    |               | <b>typical:</b> |                             |
| 10 MHz to 45 MHz                   |               | 0.5 dB          | 2 dB                        |
| 45 MHz to 500 MHz                  |               | 0.5 dB          | 0.5 dB                      |
| 500 MHz to 2 GHz                   |               | 0.5 dB          | 0.5 dB                      |
| 2 GHz to 5 GHz                     |               | 1.5 dB          | 0.5 dB                      |
| 5 GHz to 10 GHz                    |               | 1.5 dB          | 0.5 dB                      |
| 10 GHz to 24 GHz                   |               | 2 dB            | 1 dB                        |
| 24 GHz to 30 GHz                   |               | 2.5 dB          | 1 dB                        |
| 30 GHz to 40 GHz                   |               | 3 dB            | 1 dB                        |
| 40 GHz to 45 GHz                   |               | 3 dB            | 1 dB                        |
| 45 GHz to 50 GHz                   |               | 3.5 dB          | 1 dB                        |
| 50 GHz to 60 GHz                   |               | 4 dB            | 1.5 dB                      |
| 60 GHz to 67 GHz                   |               | 4.5 dB          | 2.00 dB                     |

|                         |  |          |         |
|-------------------------|--|----------|---------|
| 67 GHz to 70 GHz        |  | 6 dB     | 3.50 dB |
| <b>Damage Level</b>     |  |          |         |
| E8361A                  |  | + 27 dBm |         |
| <b>Maximum DC Level</b> |  |          |         |
| E8361A                  |  | +/- 40 V |         |

**Table 28:** Coupler Outputs (Port 1 Cplr Arm, Port 2 Cplr Arm)

| Description             | Specification | Supplemental Information |
|-------------------------|---------------|--------------------------|
| <b>Damage Level</b>     |               |                          |
| E8361A                  |               | + 30 dBm                 |
| <b>Maximum DC Level</b> |               |                          |
| E8361A                  |               | +/- 7 V                  |


## Specifications: Front-Panel Jumpers

---

### Model N5230A Options 025, 125, 225, 425, and 525

---

**NOTE:** The N5230A Options 020, 120, 220, 420, and 520 (Standard Test Set and Standard Power Range) have no front-panel jumpers.

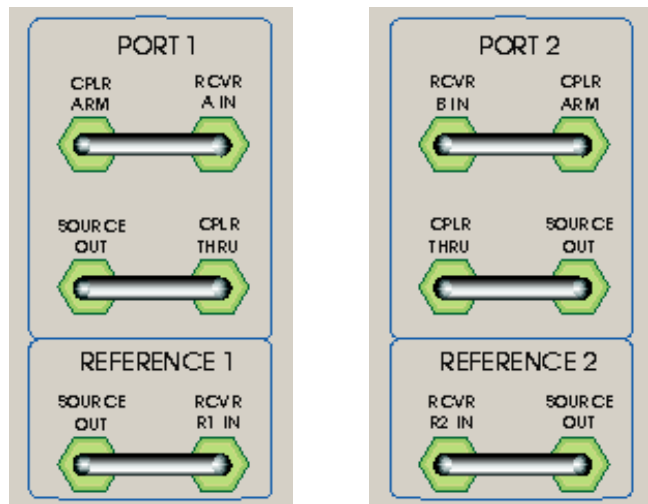

**Measurement Receiver Inputs (Rcvr A In, Rcvr B In)**

**Reference Receiver Inputs (Rcvr R1 In, Rcvr R2 In)**

**Reference Outputs (Reference 1 Source Out, Reference 2 Source Out)**

**Source Outputs (Port 1 Source Out, Port 2 Source Out)**

**Coupler Inputs (Port 1 Coupler Thru, Port 2 Coupler Thru)**

**Coupler Outputs (Port 1 Coupler Arm, Port 2 Coupler Arm)**

---

**Table 30:** Measurement Receiver Inputs (Rcvr A In, Rcvr B In) 0.1dB Typical Compression

| Description                | Specification | Typical            |            |                  |
|----------------------------|---------------|--------------------|------------|------------------|
|                            |               | Option 025,<br>125 | Option 225 | Options 425, 525 |
| <b>Maximum Input Level</b> |               |                    |            |                  |
| 300 kHz to 10 MHz          | --            | -11 dBm            | --         | --               |
| 10 MHz to 45 MHz           | --            | -7 dBm             | - 2 dBm    | - 20 dBm         |
| 45 MHz to 500 MHz          | --            | -7 dBm             | - 2 dBm    | - 19 dBm         |
| 500 MHz to 2 GHz           | --            | -6 dBm             | - 3 dBm    | - 14 dBm         |
| 2 GHz to 12.5 GHz          | --            | -6 dBm             | - 6 dBm    | - 14 dBm         |
| 12.5 GHz to 13.5 GHz       | --            | -7 dBm             | - 6 dBm    | - 15 dBm         |
| 13.5 GHz to 20 GHz         | --            | --                 | - 6 dBm    | - 15 dBm         |
| 20 GHz to 31.25 GHz        | --            | --                 | --         | - 16 dBm         |
| 31.25 GHz to 40 GHz        | --            | --                 | --         | - 21 dBm         |
| 40 GHz to 45 GHz           | --            | --                 | --         | - 24 dBm         |
| 45 GHz to 50 GHz           | --            | --                 | --         | - 22 dBm         |
| <b>Damage Level</b>        |               |                    |            |                  |
| N5230A                     | --            | + 15 dBm           |            |                  |
| <b>Maximum DC Level</b>    |               |                    |            |                  |
| N5230A                     | --            | +/- 16 V           | +/- 7 V    |                  |

**Table 31:** Reference Receiver Inputs (Rcvr R1, Rcvr R2) @ Max Specified Output Power



| Description                | Specification | Typical         |            |                  |
|----------------------------|---------------|-----------------|------------|------------------|
|                            |               | Option 025, 125 | Option 225 | Options 425, 525 |
| <b>Maximum Input Level</b> |               |                 |            |                  |
| 300 kHz to 10 MHz          | --            | -15 dBm         | --         | --               |
| 10 MHz to 500 MHz          | --            | -13 dBm         | - 18 dBm   | - 28 dBm         |
| 500 MHz to 2 GHz           | --            | -14 dBm         | - 18 dBm   | - 28 dBm         |
| 2 GHz to 6 GHz             | --            | -14 dBm         | - 19 dBm   | - 28 dBm         |
| 6 GHz to 8 GHz             | --            | -16 dBm         | - 19 dBm   | - 28 dBm         |
| 8 GHz to 9 GHz             | --            | -16 dBm         | - 21 dBm   | - 27 dBm         |
| 9 GHz to 10.5 GHz          | --            | -20 dBm         | - 21 dBm   | - 27 dBm         |
| 10.5 GHz to 12.5 GHz       | --            | -22 dBm         | - 21 dBm   | - 27 dBm         |
| 12.5 GHz to 13.5 GHz       | --            | -24 dBm         | - 23 dBm   | - 26 dBm         |
| 13.5 GHz to 20 GHz         | --            | --              | - 23 dBm   | - 26 dBm         |
| 20 GHz to 31.25 GHz        | --            | --              | --         | - 33 dBm         |
| 31.25 GHz to 40 GHz        | --            | --              | --         | - 27 dBm         |
| 40 GHz to 45 GHz           | --            | --              | --         | - 29 dBm         |
| 45 GHz to 50 GHz           | --            | --              | --         | - 28 dBm         |
| <b>Damage Level</b>        |               |                 |            |                  |
| N5230A                     | --            | + 15 dBm        |            |                  |
| <b>Maximum DC Level</b>    |               |                 |            |                  |
| N5230A                     | --            | +/- 16 V        | +/- 7 V    |                  |

**Table 32:** Reference Outputs (Reference 1 Source Out, Reference 2 Source Out) @ Max Specified Output Power

| Description                | Specification | Typical         |            |                  |
|----------------------------|---------------|-----------------|------------|------------------|
|                            |               | Option 025, 125 | Option 225 | Options 425, 525 |
| <b>Maximum Input Level</b> |               |                 |            |                  |
| 300 kHz to 10 MHz          | --            | -15 dBm         | --         | --               |
| 10 MHz to 500 MHz          | --            | -13 dBm         | - 18 dBm   | - 28 dBm         |
| 500 MHz to 2 GHz           | --            | -14 dBm         | - 18 dBm   | - 28 dBm         |
| 2 GHz to 6 GHz             | --            | -14 dBm         | - 19 dBm   | - 28 dBm         |
| 6 GHz to 8 GHz             | --            | -16 dBm         | - 19 dBm   | - 28 dBm         |
| 8 GHz to 9 GHz             | --            | -16 dBm         | - 20 dBm   | - 27 dBm         |
| 9 GHz to 10.5 GHz          | --            | -20 dBm         | - 20 dBm   | - 27 dBm         |
| 10.5 GHz to 12.5 GHz       | --            | -22 dBm         | - 20 dBm   | - 27 dBm         |
| 12.5 GHz to 13.5 GHz       | --            | -24 dBm         | - 23 dBm   | - 26 dBm         |
| 13.5 GHz to 20 GHz         | --            | --              | - 23 dBm   | - 26 dBm         |
| 20 GHz to 31.25 GHz        | --            | --              | --         | - 32 dBm         |
| 31.25 GHz to 40 GHz        | --            | --              | --         | - 26 dBm         |
| 40 GHz to 45 GHz           | --            | --              | --         | - 29 dBm         |
| 45 GHz to 50 GHz           | --            | --              | --         | - 28 dBm         |
| <b>Damage Level</b>        |               |                 |            |                  |
| N5230A                     | --            | + 20 dBm        |            |                  |
| <b>Maximum DC Level</b>    |               |                 |            |                  |
| N5230A                     | --            | +/- 16 V        | +/- 7 V    |                  |

**Table 33:** Source Outputs (Port 1 Source Out, Port 2 Source Out) @ Max Specified Output Power

| Description                | Specification | Typical            |            |                  |
|----------------------------|---------------|--------------------|------------|------------------|
|                            |               | Option 025,<br>125 | Option 225 | Options 425, 525 |
| <b>Maximum Input Level</b> |               |                    |            |                  |
| 300 kHz to 10 MHz          | --            | +11 dBm            | --         | --               |
| 10 MHz to 500 MHz          | --            | +11 dBm            | + 6 dBm    | +1 dBm           |
| 500 MHz to 6 GHz           | --            | +11 dBm            | +7 dBm     | +1 dBm           |
| 6 GHz to 9 GHz             | --            | +10 dBm            | +7 dBm     | +1 dBm           |
| 9 GHz to 12.5 GHz          | --            | +8 dBm             | +7 dBm     | +1 dBm           |
| 12.5 GHz to 13.5 GHz       | --            | +5 dBm             | +5 dBm     | +3 dBm           |
| 13.5 GHz to 20 GHz         | --            | --                 | +5 dBm     | +3 dBm           |
| 20 GHz to 31.25 GHz        | --            | --                 | --         | -5 dBm           |
| 31.25 GHz to 40 GHz        | --            | --                 | --         | -4 dBm           |
| 40 GHz to 45 GHz           | --            | --                 | --         | - 11 dBm         |
| 45 GHz to 50 GHz           | --            | --                 | --         | - 11 dBm         |
| <b>Damage Level</b>        |               |                    |            |                  |
| N5230A                     | --            | + 27 dBm           | + 30 dBm   |                  |
| <b>Maximum DC Level</b>    |               |                    |            |                  |
| N5230A                     | --            | +/- 16 V           | +/- 7 V    |                  |

**Table 34:** Coupler Inputs (Port 1 Cplr Thru, Port 2 Cplr Thru) Insertion Loss of Coupler Thru

| Description                | Specification | Typical         |            |                  |
|----------------------------|---------------|-----------------|------------|------------------|
|                            |               | Option 025, 125 | Option 225 | Options 425, 525 |
| <b>Maximum Input Level</b> |               |                 |            |                  |
| 300 kHz to 10 MHz          | --            | 2 dB            | --         | --               |
| 10 MHz to 500 MHz          | --            | 2 dB            | 0.6 dB     | 0.6 dB           |
| 500 MHz to 2 GHz           | --            | 3 dB            | 1.6 dB     | 0.8 dB           |
| 2 GHz to 8 GHz             | --            | 3 dB            | 1.8 dB     | 1 dB             |
| 8 GHz to 9 GHz             | --            | 3 dB            | 1.9 dB     | 1 dB             |
| 9 GHz to 12.5 GHz          | --            | 4 dB            | 1.9 dB     | 1 dB             |
| 12.5 GHz to 13.5 GHz       | --            | 4 dB            | 2.0 dB     | 2 dB             |
| 13.5 GHz to 20 GHz         | --            | --              | 2.0 dB     | 2 dB             |
| 20 GHz to 31.25 GHz        | --            | --              | --         | 3 dB             |
| 31.25 GHz to 50 GHz        | --            | --              | --         | 4 dB             |
| <b>Damage Level</b>        |               |                 |            |                  |
| N5230A                     | --            | + 27 dBm        | + 30 dBm   |                  |
| <b>Maximum DC Level</b>    |               |                 |            |                  |
| N5230A                     | --            | +/- 16 V        | +/- 40 V   |                  |


**Table 35:** Coupler Outputs (Port 1 Cplr Arm, Port 2 Cplr Arm)

| Description             | Specification | Typical         |            |                 |
|-------------------------|---------------|-----------------|------------|-----------------|
|                         |               | Option 025, 125 | Option 225 | Option 425, 525 |
| <b>Damage Level</b>     |               |                 |            |                 |
| N5230A                  | --            | + 15 dBm        | + 30 dBm   |                 |
| <b>Maximum DC Level</b> |               |                 |            |                 |
| N5230A                  | --            | 0 V             | +/- 7 V    |                 |

## Specifications: Front-Panel Jumpers

### Model N5230A Option 245

**Note:** The N5230A Option 240 (Standard Test Set and Standard Power Range) has no front-panel jumpers.

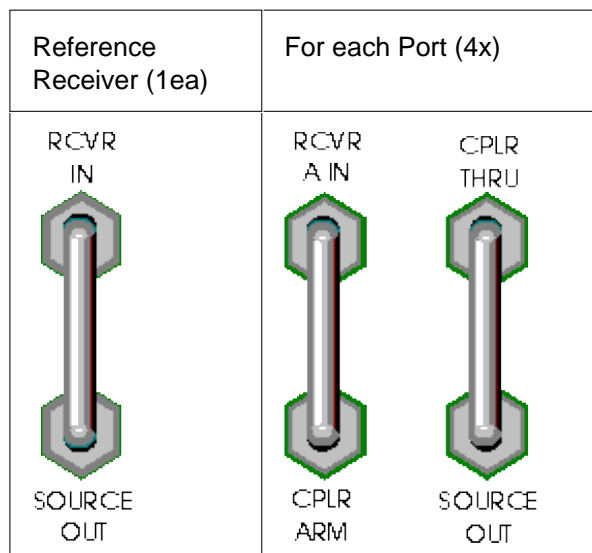

(See block diagram)

**Measurement Receiver Inputs (Rcvr A In, Rcvr B In, Rcvr C In, Rcvr D In)**

**Reference Receiver Inputs (Rcvr In)**

**Reference Outputs (Source Out)**

**Source Outputs (Port 1 Source Out, Port 2 Source Out, Port 3 Source Out, Port 4 Source Out)**

**Coupler Inputs (Port 1 Coupler Thru, Port 2 Coupler Thru, Port 3 Coupler Thru, Port 4 Coupler Thru)**

**Coupler Outputs (Port 1 Coupler Arm, Port 2 Coupler Arm)**

**Table 20:** Measurement Receiver Inputs (Rcvr A In, Rcvr B In, Rcvr C In, Rcvr D In) 0.1dB Typical Compression

| Description                | Specification | Typical           |
|----------------------------|---------------|-------------------|
|                            |               | <b>Option 245</b> |
| <b>Maximum Input Level</b> |               |                   |
| 300 kHz to 10 MHz          | --            | - 11 dBm          |
| 10 MHz to 1 GHz            | --            | - 7 dBm           |
| 1 GHz to 12.5 GHz          | --            | - 6 dBm           |
| 12.5 GHz to 20 GHz         | --            | - 7 dBm           |
| <b>Damage Level</b>        |               |                   |
| N5230A                     | --            | + 15 dBm          |
| <b>Maximum DC Level</b>    |               |                   |
| N5230A                     | --            | +/- 16 V          |

**Table 21:** Reference Receiver Input (Rcvr In) @ Max Specified Output Power

| Description                | Specification | Typical           |
|----------------------------|---------------|-------------------|
|                            |               | <b>Option 245</b> |
| <b>Maximum Input Level</b> |               |                   |
| 300 kHz to 10 MHz          | --            | - 15 dBm          |
| 10 MHz to 45 MHz           | --            | - 15 dBm          |
| 45 MHz to 500 MHz          | --            | - 15 dBm          |
| 500 MHz to 4 GHz           | --            | - 15 dBm          |
| 4 GHz to 6 GHz             | --            | - 16 dBm          |
| 6 GHz to 10.5 GHz          | --            | - 20 dBm          |
| 10.5 GHz to 15 GHz         | --            | - 21 dBm          |
| 15 GHz to 20 GHz           | --            | - 27 dBm          |
| <b>Damage Level</b>        |               |                   |
| N5230A                     | --            | + 15 dBm          |
| <b>Maximum DC Level</b>    |               |                   |
| N5230A                     | --            | +/- 16 V          |

**Table 22: Reference Output (Source Out) @ Max Specified Output Power**

| Description                 | Specification | Typical           |
|-----------------------------|---------------|-------------------|
|                             |               | <b>Option 245</b> |
| <b>Maximum Output Level</b> |               |                   |
| 300 kHz to 10 MHz           | --            | - 15 dBm          |
| 10 MHz to 45 MHz            | --            | - 15 dBm          |
| 45 MHz to 500 MHz           | --            | - 15 dBm          |
| 500 MHz to 4 GHz            | --            | - 15 dBm          |
| 4 GHz to 6 GHz              | --            | - 15 dBm          |
| 6 GHz to 10.5 GHz           | --            | - 20 dBm          |
| 10.5 GHz to 15 GHz          | --            | - 21 dBm          |
| 15 GHz to 20 GHz            | --            | - 27 dBm          |
| <b>Damage Level</b>         |               |                   |
| N5230A                      | --            | + 27 dBm          |
| <b>Maximum DC Level</b>     |               |                   |
| N5230A                      | --            | +/- 16 V          |

**Table 23: Source Outputs (Port 1 Source Out, Port 2 Source Out, Port 3 Source Out, Port 4 Source Out) @ Max Specified Output Power**

| Description                 | Specification | Typical           |
|-----------------------------|---------------|-------------------|
|                             |               | <b>Option 245</b> |
| <b>Maximum Output Level</b> |               |                   |
| 300 kHz to 10 MHz           | --            | +10 dBm           |
| 10 MHz to 45 MHz            | --            | + 10 dBm          |
| 45 MHz to 500 MHz           | --            | + 10 dBm          |
| 500 MHz to 4 GHz            | --            | + 10 dBm          |
| 4 GHz to 6 GHz              | --            | + 9 dBm           |
| 6 GHz to 10.5 GHz           | --            | + 4 dBm           |

|                         |    |          |
|-------------------------|----|----------|
| 10.5 GHz to 15 GHz      | -- | + 1 dBm  |
| 15 GHz to 20 GHz        | -- | - 4 dBm  |
| <b>Damage Level</b>     |    |          |
| N5230A                  | -- | + 27 dBm |
| <b>Maximum DC Level</b> |    |          |
| N5230A                  | -- | +/- 16V  |

**Table 24:** Coupler Inputs (Port 1 Cplr Thru, Port 2 Cplr Thru, Port 3 Cplr Thru, Port 4 Cplr Thru)  
Insertion Loss of Coupler Thru

| Description                        | Specification | Typical           |
|------------------------------------|---------------|-------------------|
|                                    |               | <b>Option 245</b> |
| <b>Insertion Loss to Test Port</b> |               |                   |
| 300 kHz to 10 MHz                  |               | 1.5 dB            |
| 10 MHz to 45 MHz                   | --            | 1.5 dB            |
| 45 MHz to 500 MHz                  | --            | 1.5 dB            |
| 500 MHz to 4 GHz                   | --            | 2.0 dB            |
| 4 GHz to 6 GHz                     | --            | 2.5 dB            |
| 6 GHz to 10.5 GHz                  | --            | 2.5 dB            |
| 10.5 GHz to 15 GHz                 | --            | 3.0 dB            |
| 15 GHz to 20 GHz                   | --            | 3.0 dB            |
| <b>Damage Level</b>                |               |                   |
| N5230A                             | --            | + 27 dBm          |
| <b>Maximum DC Level</b>            |               |                   |
| N5230A                             | --            | +/- 16 V          |

**Table 25:** Coupler Outputs (Port 1 Cplr Arm, Port 2 Cplr Arm, Port 3 Cplr Arm, Port 4 Cplr Arm)



| Description             | Specification | Typical           |
|-------------------------|---------------|-------------------|
|                         |               | <b>Option 245</b> |
| <b>Damage Level</b>     |               |                   |
| N5230A                  | --            | + 15 dBm          |
| <b>Maximum DC Level</b> |               |                   |
| N5230A                  | --            | 0 V               |

## Specifications: Front-Panel Jumpers

---


### Models E8356A, E8357A, E8358A - Standard

- Port 1
- Port 2

### Models E8356A, E8357A, E8358A - Option 015

- Port 1
  - Port 2
- 

### E8356A, 57A, 58A, Standard - Port 1

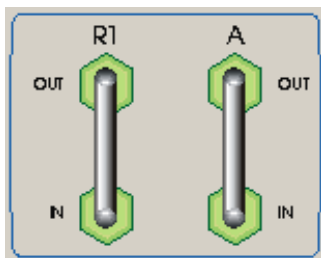

Use these SMA (female) connectors to develop custom measurements.

### Receiver A Direct-Access Jumper

- The upper "A" connector comes from the coupled arm of the Port 1 coupler.
- The lower connector goes directly to the input of receiver "A." If Option 015 is installed, the path goes directly to a switchable attenuator and then to the receiver input.

Want to upgrade your analyzer? See information on Front-Panel Jumpers with Option 015.

### For the A Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <-130 dBm (300 kHz to 25 MHz)
- <-123 dBm (3 GHz to 6 GHz)
- <-123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

- >17 dB (300 kHz to 3 GHz)
- >12 dB (3 GHz to 6 GHz)
- >7 dB (6 GHz to 9 GHz)

### Reference Channel R1 Jumper

- The upper connector comes from the transfer switch Reference 1 output.
- The lower connector goes directly to the R1 receiver input.

#### For the R1 Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Damage Level: >+15 dBm

Minimum Level to Maintain Phase-Lock:

- 35 dBm (300 kHz to 3 GHz)
- 25 dBm (3 GHz to 9 GHz)

#### For the Reference Output: (with an External Input to Lock the Source)

Output Level:

- 5 to –30 dBm (300 kHz to 6 GHz)
- 10 to –35 dBm (6 GHz to 9 GHz)

Source Match Return Loss:


- 16 dB (300 kHz to 3 GHz)
- 14 dB (3 GHz to 9 GHz)

Damage Level: >+15 dBm

Maximum DC Level: 40V

---

#### E8356A, 57A, 58A, Standard - Port 2

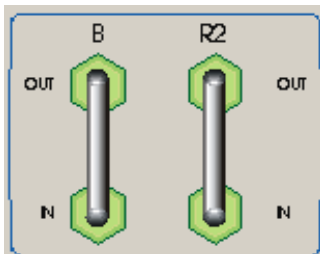

Use these SMA (female) connectors to develop custom measurements.

#### Receiver B Direct-Access Jumper

- The upper "B" connector comes from the coupled arm of the Port 2 coupler.
- The lower connector goes directly to the input of receiver "B." If Option 015 is installed, the path goes directly to a switchable attenuator and then to the receiver input.

Want to upgrade your analyzer? See information on Front-Panel Jumpers with Option 015.

#### For the B Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <–130 dBm (300 kHz to 25 MHz)

<-123 dBm (3 GHz to 6 GHz)  
<-123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

>17 dB (300 kHz to 3 GHz)  
>12 dB (3 GHz to 6 GHz)  
>7 dB (6 GHz to 9 GHz)

#### Reference Channel R2 Jumper

- The upper connector comes from the transfer switch Reference 2 output.
- The lower connector goes directly to the R2 receiver input.

#### For the R2 Receiver Input:

Maximum Input Level:

-6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)  
-6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)  
-11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Damage Level: >+15 dBm

Minimum Level to Maintain Phase-Lock:

-35 dBm (300 kHz to 3 GHz)  
-25 dBm (3 GHz to 9 GHz)

#### For the Reference Output: (with an External Input to Lock the Source)

Output Level:

-5 to -30 dBm (300 kHz to 6 GHz)  
-10 to -35 dBm (6 GHz to 9 GHz)

Source Match Return Loss:


16 dB (300 kHz to 3 GHz)  
14 dB (3 GHz to 9 GHz)

Damage Level: >+15 dBm

Maximum DC Level: 40V

---

#### E8356A, 57A, 58A, Option 015 - Port 1

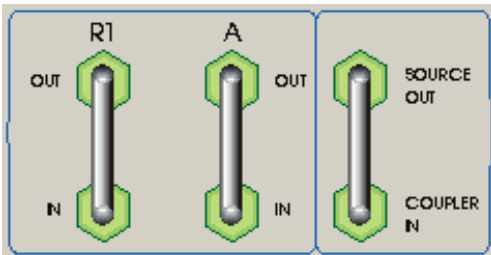

Use these SMA (female) connectors to develop custom measurements.

#### Receiver A Direct-Access Jumper

- The upper "A" connector comes from the coupled arm of the Port 1 coupler.
- The lower connector goes directly to the input of receiver "A." With Option 015, the path goes directly to a

switchable attenuator and then to the receiver input.

### **For the A Receiver Input:**

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <-130 dBm (300 kHz to 25 MHz)
- <-123 dBm (3 GHz to 6 GHz)
- <-123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

- >17 dB (300 kHz to 3 GHz)
- >12 dB (3 GHz to 6 GHz)
- >7 dB (6 GHz to 9 GHz)

### **Reference Channel R1 Jumper**

- The upper connector comes from the transfer switch Reference 1 output.
- The lower connector goes directly to the R1 receiver input.

### **For the R1 Receiver Input:**

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Damage Level: >+15 dBm

Minimum Level to Maintain Phase-Lock:

- 35 dBm (300 kHz to 3 GHz)
- 25 dBm (3 GHz to 9 GHz)

### **For the Reference Output: (with an External Input to Lock the Source)**

Output Level:

- 5 to -30 dBm (300 kHz to 6 GHz)
- 10 to -35 dBm (6 GHz to 9 GHz)

Source Match Return Loss:

- 16 dB (300 kHz to 3 GHz)
- 14 dB (3 GHz to 9 GHz)

Damage Level: >+15 dBm

Maximum DC Level: 40V

### **Port 1 Test-Port Jumper**

- The upper "source out" connector comes from the transfer switch Port 1 output.
- The lower "coupler in" connector goes directly to the main input of Port 1 coupler. This is where a power amplifier can be inserted to boost the test port power.

### For the Source Output:

Output Level:

+12 to -83 dBm (300 kHz to 6 GHz)

+7 to -88 dBm (6 GHz to 9 GHz)

Source Match: 15 dB at 9 GHz

### For the Input to the Coupler:

Insertion Loss to Test Port 1:

<3.5 dB at 3 GHz


<5 dB at 9 GHz

Maximum Input Power: 2 Watts, CW

Damage Level: 4 Watts, CW

---

### E8356A, 57A, 58A, Option 015 - Port 2

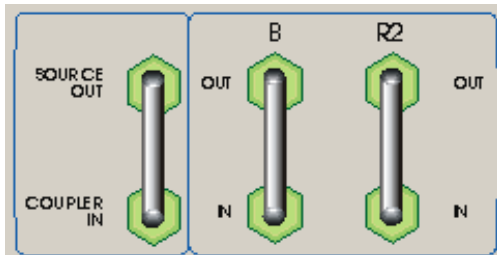

Use these SMA (female) connectors to develop custom measurements.

### Receiver B Direct-Access Jumper

- The upper "B" connector comes from the coupled arm of the Port 2 coupler.
- The lower connector goes directly to the input of receiver "B." With Option 015, the path goes directly to a switchable attenuator and then to the receiver input.

### For the B Receiver Input:

Maximum Input Level:

-6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)

-6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)

-11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

<-130 dBm (300 kHz to 25 MHz)

<-123 dBm (3 GHz to 6 GHz)

<-123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

>17 dB (300 kHz to 3 GHz)

>12 dB (3 GHz to 6 GHz)

>7 dB (6 GHz to 9 GHz)

### Reference Channel R2 Jumper

- The upper connector comes from the transfer switch Reference 2 output.

- The lower connector goes directly to the R2 receiver input.

### **For the R2 Receiver Input:**

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Damage Level: >+15 dBm

Minimum Level to Maintain Phase-Lock:

- 35 dBm (300 kHz to 3 GHz)
- 25 dBm (3 GHz to 9 GHz)

### **For the Reference Output: (with an External Input to Lock the Source)**

Output Level:

- 5 to -30 dBm (300 kHz to 6 GHz)
- 10 to -35 dBm (6 GHz to 9 GHz)

Source Match Return Loss:

- 16 dB (300 kHz to 3 GHz)
- 14 dB (3 GHz to 9 GHz)

Damage Level: >+15 dBm

Maximum DC Level: 40V

### **Port 2 Test-Port Jumper**

- The upper "source out" connector comes from the transfer switch Port 2 output.
- The lower "coupler in" connector goes directly to the main input of Port 2 coupler. This is where a power amplifier can be inserted to boost the test port power.

### **For the Source Output:**

Output Level:

- +12 to -83 dBm (300 kHz to 6 GHz)
- +7 to -88 dBm (6 GHz to 9 GHz)

Source Match: 15 dB at 9 GHz

### **For the Input to the Coupler:**

Insertion Loss to Test Port 2:

- <3.5 dB at 3 GHz
- <5 dB at 9 GHz

Maximum Input Power: 2 Watts, CW

Damage Level: 4 Watts, CW

## Specifications: Front-Panel Jumpers


Models E8801A, E8802A, E8803A Option 014

### Port 1

### Port 2

---

## Specifications: Front-Panel Jumpers, Port 1

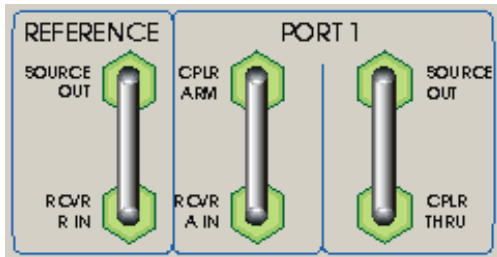

### Option 014 Analyzer

NOTE: The standard analyzer (E8801A/ E8802A/ E8803A) has no front-panel jumpers.

Use these SMA (female) connectors to develop custom measurements.

#### Receiver A Direct-Access Jumper

- The "Cplr Arm" connector comes from the coupled arm of the Port 1 coupler.
- The "Rcvr A In" connector goes directly to the input of receiver "A."

#### For the A Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <–130 dBm (300 kHz to 25 MHz)
- <–123 dBm (3 GHz to 6 GHz)
- <–123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

- >17 dB (300 kHz to 3 GHz)
- >12 dB (3 GHz to 6 GHz)
- >7 dB (6 GHz to 9 GHz)

#### Reference Channel R Jumper

- The "Source Out" connector comes from the source Reference output.
- The "Rcvr R In" connector goes directly to the R receiver input.

#### For the R Receiver Input:



Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Damage Level: >+15 dBm

Minimum Level to Maintain Phase-Lock:

- 35 dBm (300 kHz to 3 GHz)
- 25 dBm (3 GHz to 9 GHz)

**For the Reference Output: (with an External Input to Lock the Source)**

Output Level:

- 5 to -30 dBm (300 kHz to 6 GHz)
- 10 to -35 dBm (6 GHz to 9 GHz)

Source Match Return Loss:

- 16 dB (300 kHz to 3 GHz)
- 14 dB (3 GHz to 9 GHz)

Damage Level: >+15 dBm

Maximum DC Level: 40V

**Port 1 Test-Port Jumper**

- The upper "Source Out" connector comes from the transfer switch Port 1 output.
- The lower "Coupler Thru" connector goes directly to the main input of Port 1 coupler. This is where a power amplifier can be inserted to boost the test port power.

**For the Source Output:**

Output Level:

- +12 to -83 dBm (300 kHz to 6 GHz)
- +7 to -88 dBm (6 GHz to 9 GHz)

Source Match: 15 dB at 9 GHz

**For the Input to the Coupler:**

Insertion Loss to Test Port 1:


- <3.5 dB at 3 GHz
- <5 dB at 9 GHz

Maximum Input Power: 2 Watts, CW

Damage Level: 4 Watts, CW

---

**Specifications: Front-Panel Jumpers, Port 2**

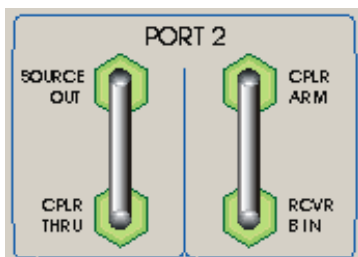

## Option 014 Analyzer

NOTE: The standard analyzer (E8801A/ E8802A/ E8803A) has no front-panel jumpers.

---

Use these SMA (female) connectors to develop custom measurements.

### Receiver B Direct-Access Jumper

- The upper "Cplr Arm" connector comes from the coupled arm of the Port 2 coupler.
- The "Rcvr B In" connector goes directly to the input of receiver "B."

### For the B Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <-130 dBm (300 kHz to 25 MHz)
- <-123 dBm (3 GHz to 6 GHz)
- <-123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

- >17 dB (300 kHz to 3 GHz)
- >12 dB (3 GHz to 6 GHz)
- >7 dB (6 GHz to 9 GHz)

### Port 2 Test-Port Jumper

- The upper "Source Out" connector comes from the transfer switch Port 2 output.
- The lower "Coupler Thru" connector goes directly to the main input of Port 2 coupler. This is where a power amplifier can be inserted to boost the test port power.

### For the Source Output:

Output Level:

- +12 to -83 dBm (300 kHz to 6 GHz)
- +7 to -88 dBm (6 GHz to 9 GHz)

Source Match: 15 dB at 9 GHz

### For the Input to the Coupler:

Insertion Loss to Test Port 2:

- <3.5 dB at 3 GHz
- <5 dB at 9 GHz

Maximum Input Power: 2 Watts, CW

Damage Level: 4 Watts, CW

## Specifications: Front-Panel Jumpers


Models N3381A, N3382A, N3383A Option 014

### Port 1

### Port 2 and Port 3

---

## Specifications: Front-Panel Jumpers, Port 1

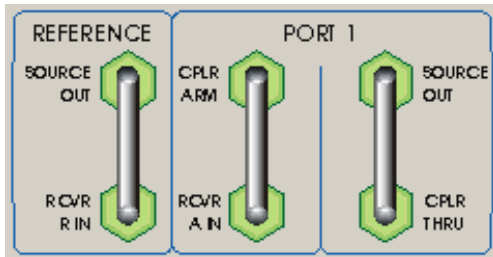

### Option 014 Analyzer

NOTE: The standard analyzer (N3381A/ N3382A/ N3383A) has no front-panel jumpers.

Use these SMA (female) connectors to develop custom measurements.

#### Receiver A Direct-Access Jumper

- The "Cplr Arm" connector comes from the coupled arm of the Port 1 coupler.
- The "Rcvr A In" connector goes directly to the input of receiver "A."

#### For the A Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <–130 dBm (300 kHz to 25 MHz)
- <–123 dBm (3 GHz to 6 GHz)
- <–123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

- >17 dB (300 kHz to 3 GHz)
- >12 dB (3 GHz to 6 GHz)
- >7 dB (6 GHz to 9 GHz)

#### Reference Channel R Jumper

- The "Source Out" connector comes from the source Reference output.
- The "Rcvr R In" connector goes directly to the R receiver input.

#### For the R Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Damage Level: >+15 dBm

Minimum Level to Maintain Phase-Lock:

- 35 dBm (300 kHz to 3 GHz)
- 25 dBm (3 GHz to 9 GHz)

For the Reference Output: (with an External Input to Lock the Source)

Output Level:

- 5 to -30 dBm (300 kHz to 6 GHz)
- 10 to -35 dBm (6 GHz to 9 GHz)

Source Match Return Loss:

- 16 dB (300 kHz to 3 GHz)
- 14 dB (3 GHz to 9 GHz)

Damage Level: >+15 dBm

Maximum DC Level: 40V

**Port 1 Test-Port Jumper**

- The upper "Source Out" connector comes from the transfer switch Port 1 output.
- The lower "Coupler Thru" connector goes directly to the main input of Port 1 coupler. This is where a power amplifier can be inserted to boost the test port power.

**For the Source Output:**

Output Level:

- +12 to -83 dBm (300 kHz to 6 GHz)
- +7 to -88 dBm (6 GHz to 9 GHz)

Source Match: 15 dB at 9 GHz

**For the Input to the Coupler:**


Insertion Loss to Test Port 1:

- <3.5 dB at 3 GHz
- <5 dB at 9 GHz

Maximum Input Power: 2 Watts, CW

Damage Level: 4 Watts, CW

**Specifications: Front-Panel Jumpers, Port 2 and Port 3**

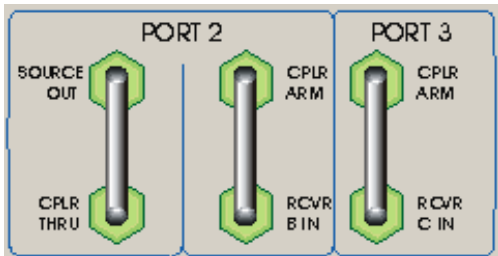

**Option 014 Analyzer**

NOTE: The standard analyzer (N3381A/ N3382A/ N3383A) has no front-panel jumpers.

---

Use these SMA (female) connectors to develop custom measurements.

#### **Receiver B Direct-Access Jumper**

- The upper "Cplr Arm" connector comes from the coupled arm of the Port 2 coupler.
- The "Rcvr B In" connector goes directly to the input of receiver "B."

For the B Receiver Input:

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <-130 dBm (300 kHz to 25 MHz)
- <-123 dBm (3 GHz to 6 GHz)
- <-123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

- >17 dB (300 kHz to 3 GHz)
- >12 dB (3 GHz to 6 GHz)
- >7 dB (6 GHz to 9 GHz)

#### **Port 2 Test-Port Jumper**

- The upper "Source Out" connector comes from the transfer switch Port 2 output.
- The lower "Coupler Thru" connector goes directly to the main input of Port 2 coupler. This is where a power amplifier can be inserted to boost the test port power.

#### **For the Source Output:**

Output Level:

- +10 to -85 dBm (300 kHz to 6 GHz)
- +7 to -88 dBm (6 GHz to 9 GHz)

Source Match: 15 dB at 9 GHz

#### **For the Input to the Coupler:**

Insertion Loss to Test Port 2:

- <3.5 dB at 3 GHz
- <5 dB at 9 GHz

Maximum Input Power: 2 Watts, CW

Damage Level: 4 Watts, CW

#### **Receiver C Direct-Access Jumper**

- The upper "Cplr Arm" connector comes from the coupled arm of the Port 3 coupler.
- The "Rcvr C In" connector goes directly to the input of receiver "C."

**For the C Receiver Input:**

Maximum Input Level:

- 6 dBm; <0.4 dB Compression (300 kHz to 3 GHz)
- 6 dBm; <0.8 dB Compression (3 GHz to 6 GHz)
- 11 dBm; <0.8 dB Compression (6 GHz to 9 GHz)

Noise Floor; rms (10 Hz Bandwidth):

- <-130 dBm (300 kHz to 25 MHz)
- <-123 dBm (6 GHz to 9 GHz)

Damage Level: +15 dBm

Maximum DC Level: +/-5 V

Return Loss:

- >17 dB (300 kHz to 3 GHz)
- >12 dB (3 GHz to 6 GHz)
- >7 dB (6 GHz to 9 GHz)

## Identify Your Analyzer

---

Please select the PNA model of the specifications you would like to see.

[<=Back](#)

Select your PNA model:

|                                                                |                                                     |                                                     |                                             |                                             |
|----------------------------------------------------------------|-----------------------------------------------------|-----------------------------------------------------|---------------------------------------------|---------------------------------------------|
| E8356A<br>E8357A<br>E8358A<br><input checked="" type="radio"/> | E8801A<br>E8802A<br>E8803A<br><input type="radio"/> | N3381A<br>N3382A<br>N3383A<br><input type="radio"/> | N5230A<br>(2-port)<br><input type="radio"/> | N5230A<br>(4-port)<br><input type="radio"/> |
| E8361A<br><input type="radio"/>                                | E8362A<br>E8363A<br>E8364A<br><input type="radio"/> | E8362B<br>E8363B<br>E8364B<br><input type="radio"/> | N5250A<br><input type="radio"/>             |                                             |

Click

## E8361A Corrected System Performance with 1.85mm Connectors

---

### 85058B Calibration Kit:

Standard Configuration and Standard Power Range (E8361A)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)

### N4694A ECal Module:

Standard Configuration and Standard Power Range (E8361A)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)

---

**Table 2.** 85058B Calibration Kit  
E8361A - Standard Configuration and Standard Power Range

Applies to the E8361A analyzers, 85058B (1.85mm) calibration kit, N4697F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB)        |                    |                    |                    |
|-----------------------|---------------------------|--------------------|--------------------|--------------------|
|                       | 10 to 45 MHz <sup>1</sup> | 45 MHz to 2 GHz    | 2 to 10 GHz        | 10 to 20 GHz       |
| Directivity           | 35                        | 35                 | 41                 | 38                 |
| Source Match          | 34                        | 34                 | 44                 | 40                 |
| Load Match            | 35                        | 35                 | 41                 | 37                 |
| Reflection Tracking   | ±0.019<br>+0.02/°C        | ±0.019<br>+0.02/°C | ±0.010<br>+0.02/°C | ±0.033<br>+0.03/°C |
| Transmission Tracking | ±0.164<br>+0.02/°C        | ±0.081<br>+0.02/°C | ±0.036<br>+0.02/°C | ±0.063<br>+0.03/°C |


<sup>1</sup> Typical performance.




| Description           | Specification (dB)                    |                                       |                                       |                                       |
|-----------------------|---------------------------------------|---------------------------------------|---------------------------------------|---------------------------------------|
|                       | 20 to 35 GHz                          | 35 to 50 GHz                          | 50 to 60 GHz                          | 60 to 67 GHz                          |
| Directivity           | 37                                    | 37                                    | 34                                    | 34                                    |
| Source Match          | 34                                    | 34                                    | 44                                    | 40                                    |
| Load Match            | 34                                    | 35                                    | 41                                    | 37                                    |
| Reflection Tracking   | $\pm 0.019$<br>$+0.02/^\circ\text{C}$ | $\pm 0.019$<br>$+0.02/^\circ\text{C}$ | $\pm 0.010$<br>$+0.02/^\circ\text{C}$ | $\pm 0.033$<br>$+0.03/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.164$<br>$+0.02/^\circ\text{C}$ | $\pm 0.081$<br>$+0.02/^\circ\text{C}$ | $\pm 0.036$<br>$+0.02/^\circ\text{C}$ | $\pm 0.063$<br>$+0.03/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

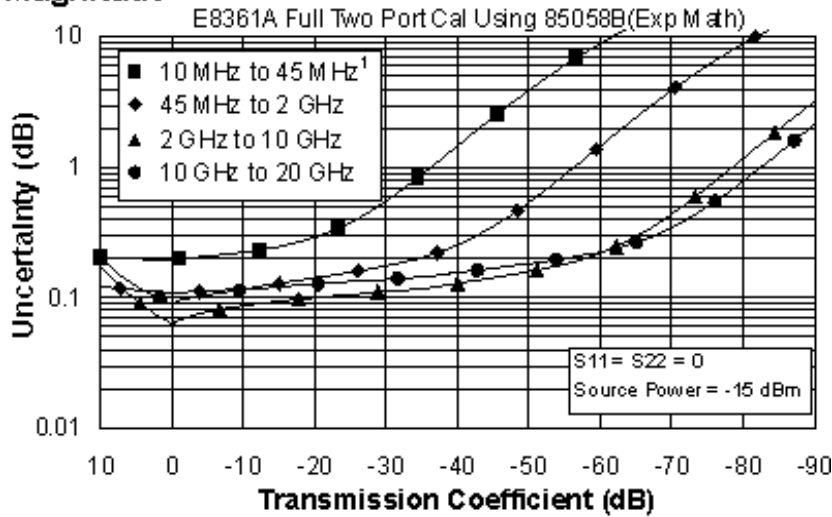


## Magnitude

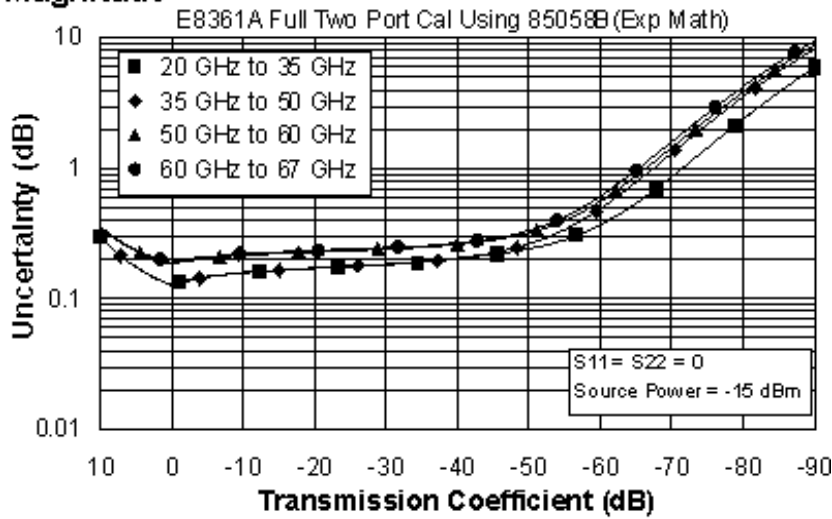


1 Typical performance.

## Phase

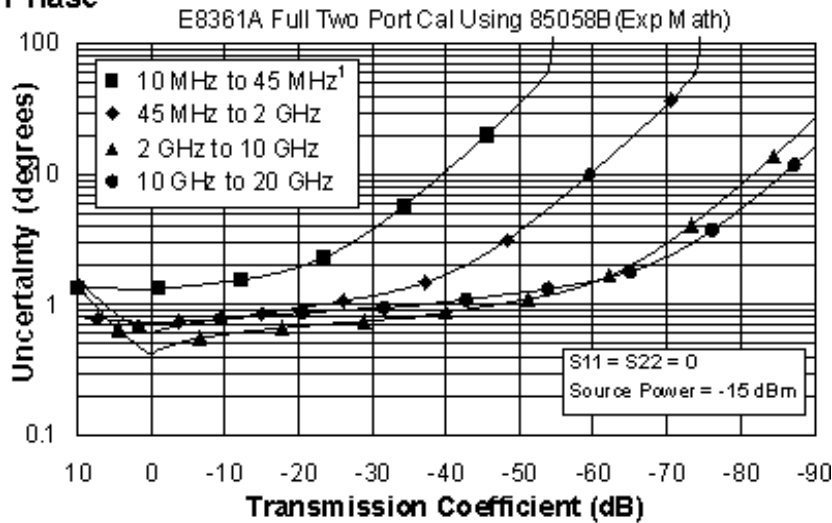


## Phase

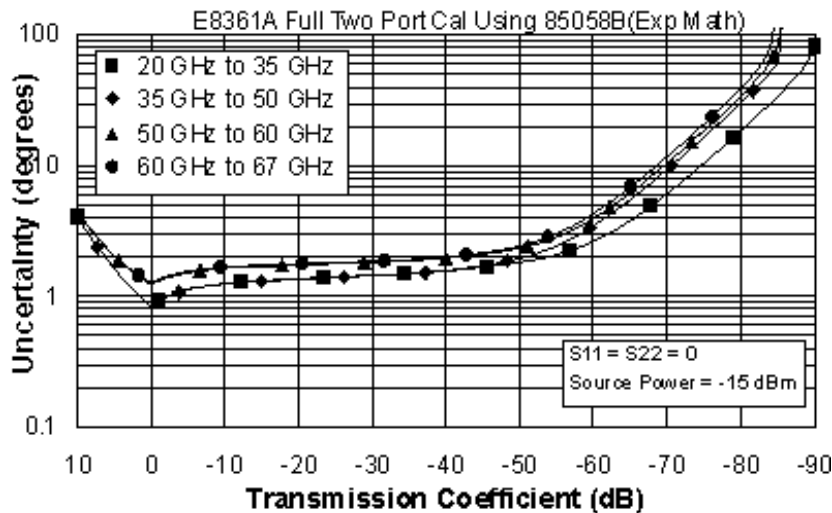


1 Typical performance.

## Reflection Uncertainty (Specifications)

### Magnitude

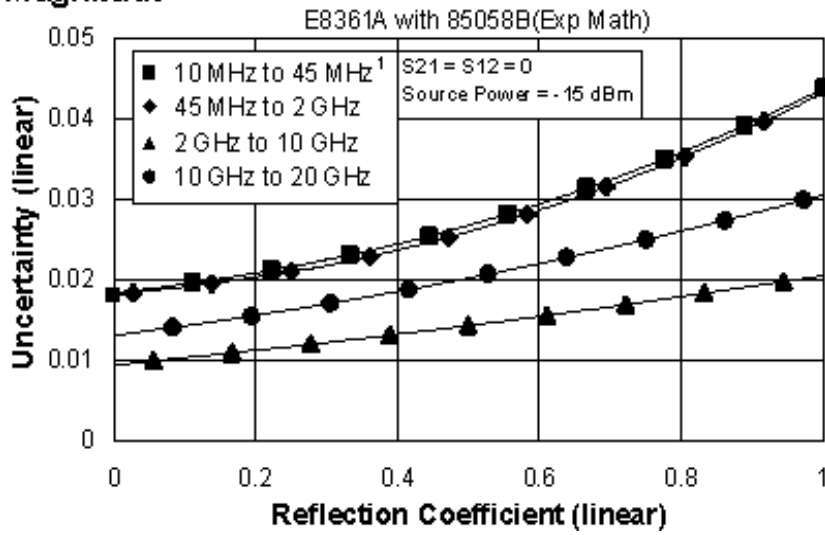


### Magnitude

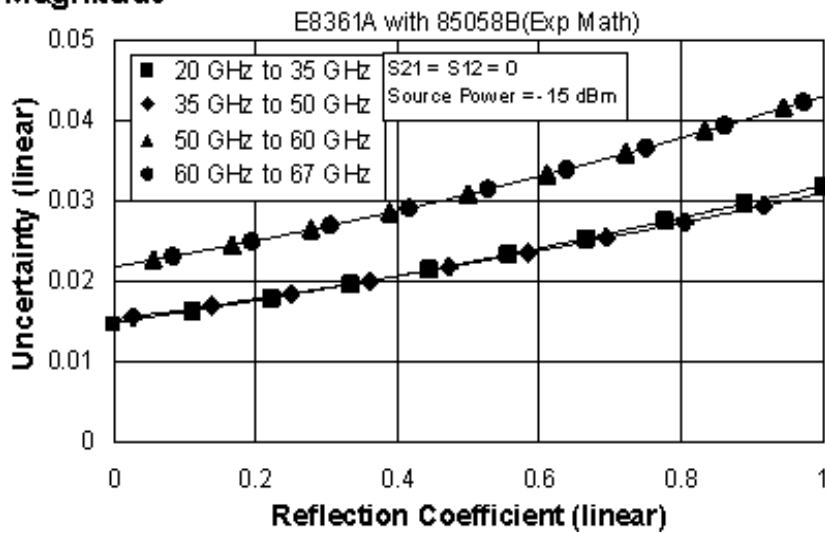


1 Typical performance.

### Phase

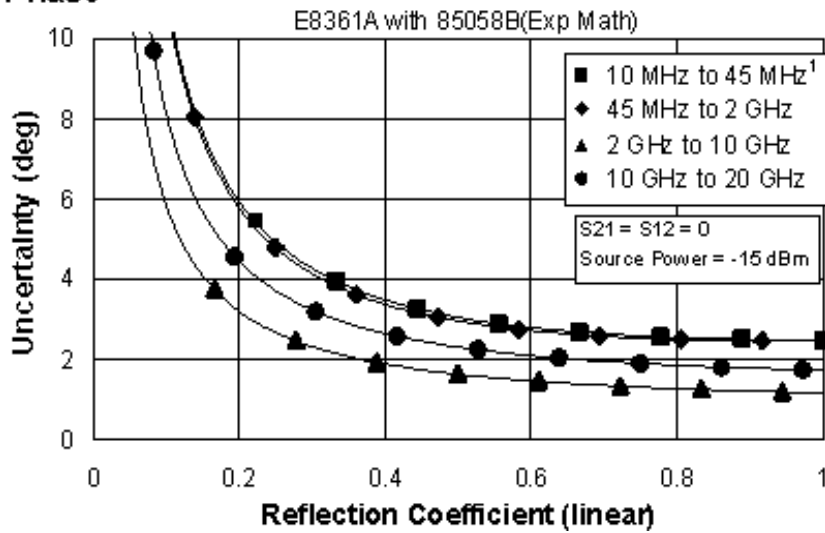

### Phase

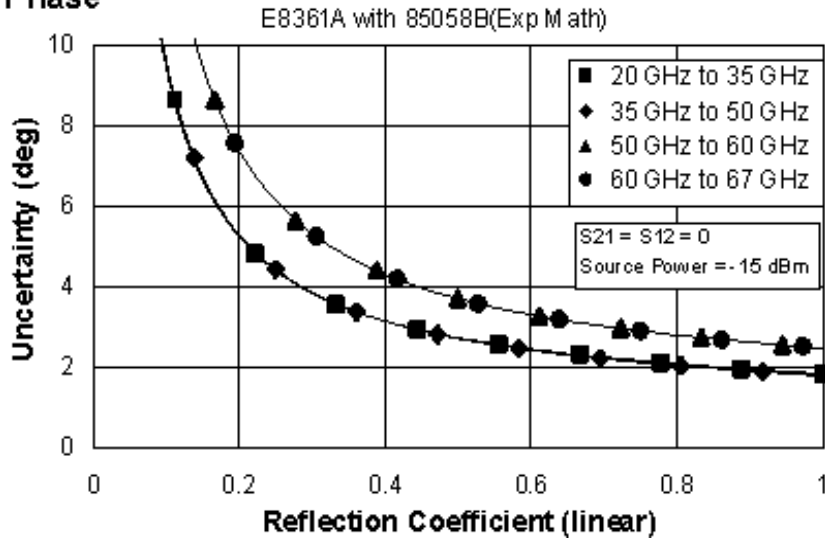

1 Typical performance.

### Table 3. 85058B Calibration Kit

E8361A - Fully Optioned (Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E8361A analyzers, 85058B (1.85mm) calibration kit, N4697F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:



Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB)        |                    |                    |                    |
|-----------------------|---------------------------|--------------------|--------------------|--------------------|
|                       | 10 to 45 MHz <sup>1</sup> | 45 MHz to 2 GHz    | 2 to 10 GHz        | 10 to 20 GHz       |
| Directivity           | 35                        | 35                 | 41                 | 38                 |
| Source Match          | 34                        | 34                 | 44                 | 40                 |
| Load Match            | 34                        | 35                 | 41                 | 37                 |
| Reflection Tracking   | ±0.019<br>+0.02/°C        | ±0.019<br>+0.02/°C | ±0.010<br>+0.02/°C | ±0.033<br>+0.03/°C |
| Transmission Tracking | ±0.177<br>+0.02/°C        | ±0.093<br>+0.02/°C | ±0.053<br>+0.02/°C | ±0.096<br>+0.03/°C |

<sup>1</sup> Typical performance.

| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 20 to 35 GHz       | 35 to 50 GHz       | 50 to 60 GHz       | 60 to 67 GHz       |
| Directivity           | 37                 | 37                 | 34                 | 34                 |
| Source Match          | 34                 | 34                 | 44                 | 40                 |
| Load Match            | 34                 | 35                 | 41                 | 37                 |
| Reflection Tracking   | ±0.019<br>+0.02/°C | ±0.019<br>+0.02/°C | ±0.010<br>+0.02/°C | ±0.033<br>+0.03/°C |
| Transmission Tracking | ±0.177<br>+0.02/°C | ±0.093<br>+0.02/°C | ±0.053<br>+0.02/°C | ±0.096<br>+0.03/°C |

### Transmission Uncertainty (Specifications)

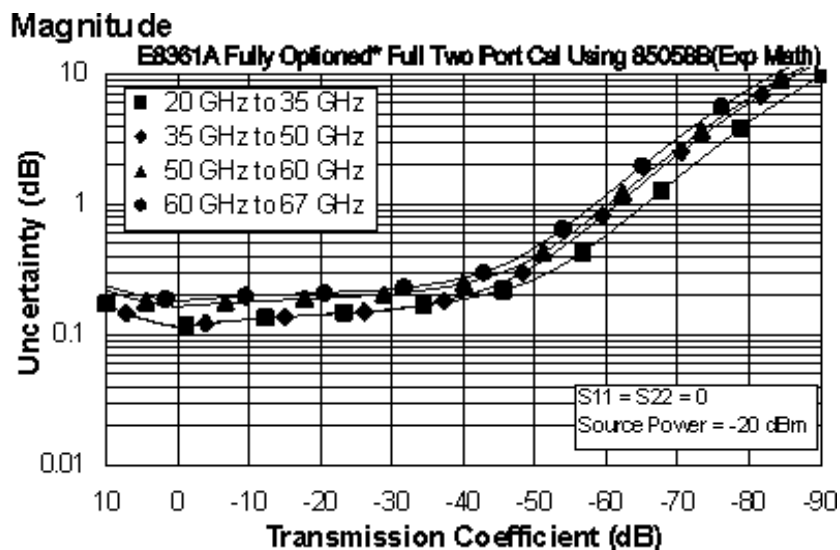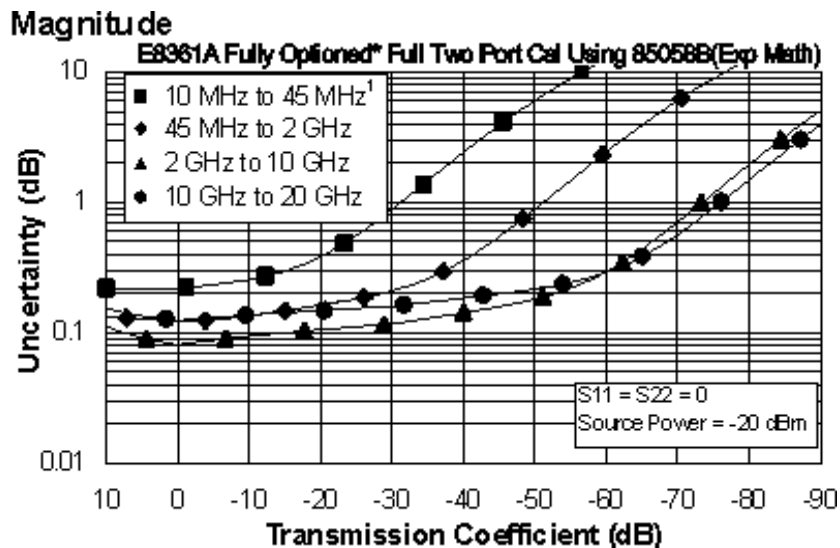


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)

1 Typical performance.


## Phase

E8361A Fully Optioned\* Full Two Port Cal Using 85058B(Exp Math)

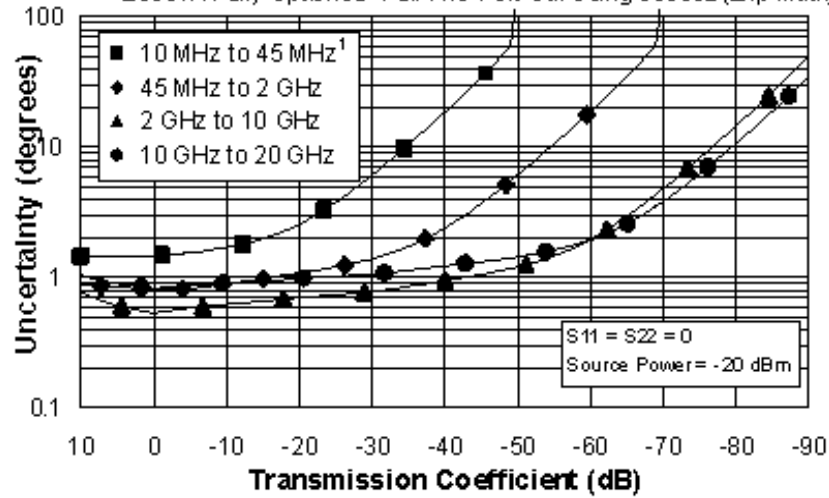

## Phase

E8361A Fully Optioned\* Full Two Port Cal Using 85058B(Exp Math)

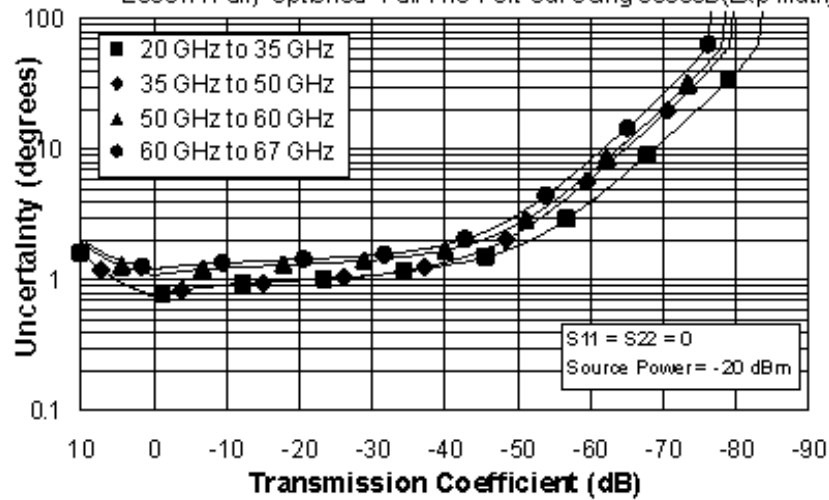


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)


<sup>1</sup> Typical performance.

## Reflection Uncertainty (Specifications)

## Magnitude

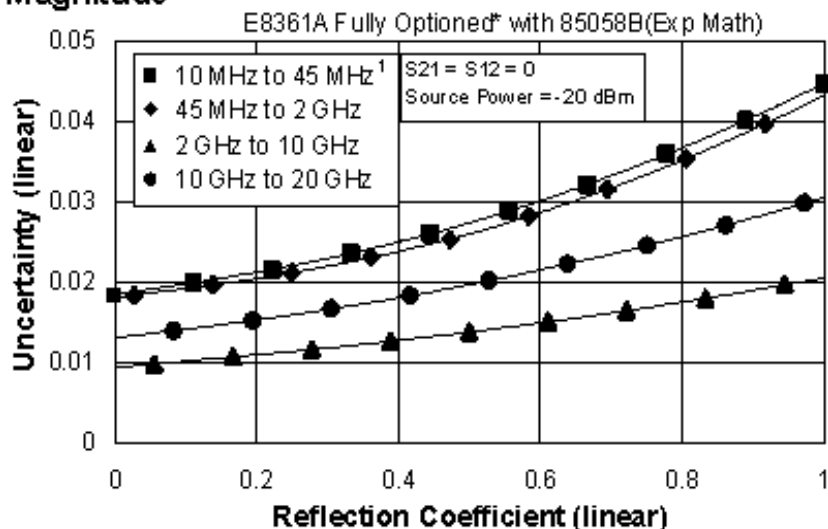



## Magnitude

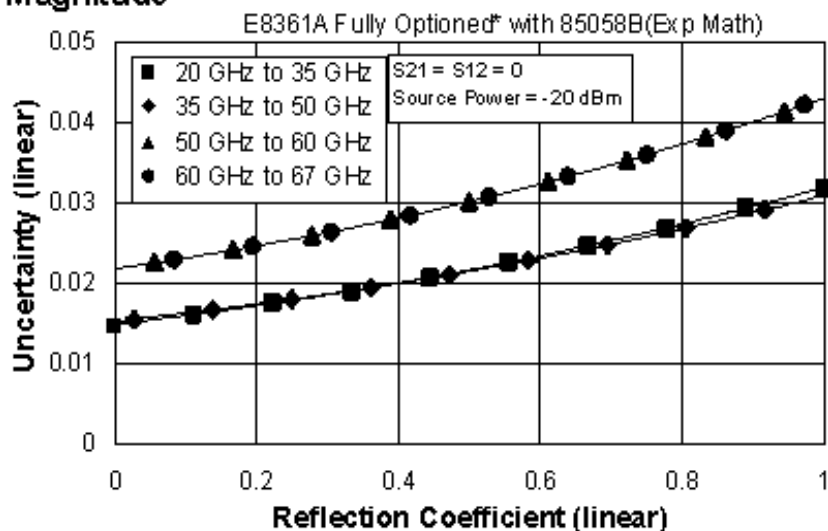

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)

<sup>1</sup> Typical performance.



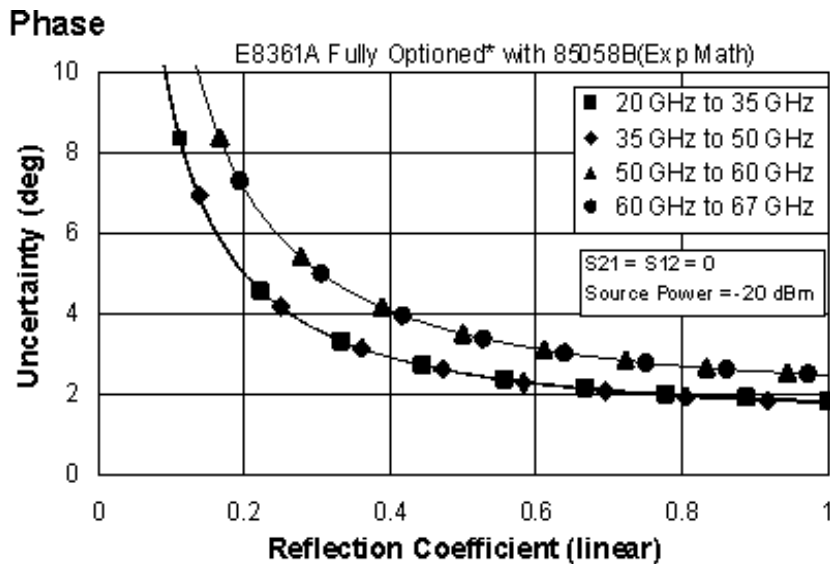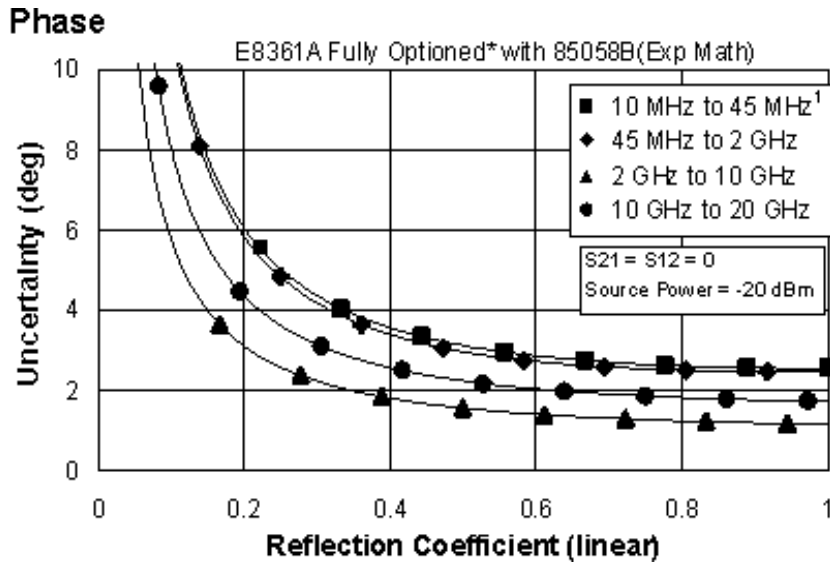

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)

<sup>1</sup> Typical performance.

**Table 4. N4694A Calibration Kit**  
 E8361A - Standard Configuration and Standard Power Range

Applies to the, E8361A analyzers, N4694A (1.85mm) ECal module, N4697F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB)        |                    |                    |                    |
|-----------------------|---------------------------|--------------------|--------------------|--------------------|
|                       | 10 to 40 MHz <sup>1</sup> | 40 MHz to 2 GHz    | 2 to 20 GHz        | 20 to 30 GHz       |
| Directivity           | 33                        | 50                 | 50                 | 46                 |
| Source Match          | 25                        | 38                 | 39                 | 35                 |
| Load Match            | 30                        | 39                 | 40                 | 38                 |
| Reflection Tracking   | ±0.050<br>+0.02/°C        | ±0.040<br>+0.02/°C | ±0.040<br>+0.02/°C | ±0.050<br>+0.03/°C |
| Transmission Tracking | ±0.255<br>+0.02/°C        | ±0.118<br>+0.02/°C | ±0.135<br>+0.02/°C | ±0.139<br>+0.03/°C |

<sup>1</sup> Typical performance.


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 30 to 40 GHz       | 40 to 50 GHz       | 50 to 60 GHz       | 60 to 67 GHz       |
| Directivity           | 44                 | 42                 | 41                 | 38                 |
| Source Match          | 25                 | 38                 | 39                 | 35                 |
| Load Match            | 30                 | 39                 | 40                 | 38                 |
| Reflection Tracking   | ±0.040<br>+0.02/°C | ±0.040<br>+0.02/°C | ±0.040<br>+0.02/°C | ±0.050<br>+0.03/°C |
| Transmission Tracking | ±0.105<br>+0.02/°C | ±0.118<br>+0.02/°C | ±0.135<br>+0.02/°C | ±0.139<br>+0.03/°C |

### Transmission Uncertainty (Specifications)

## Magnitude

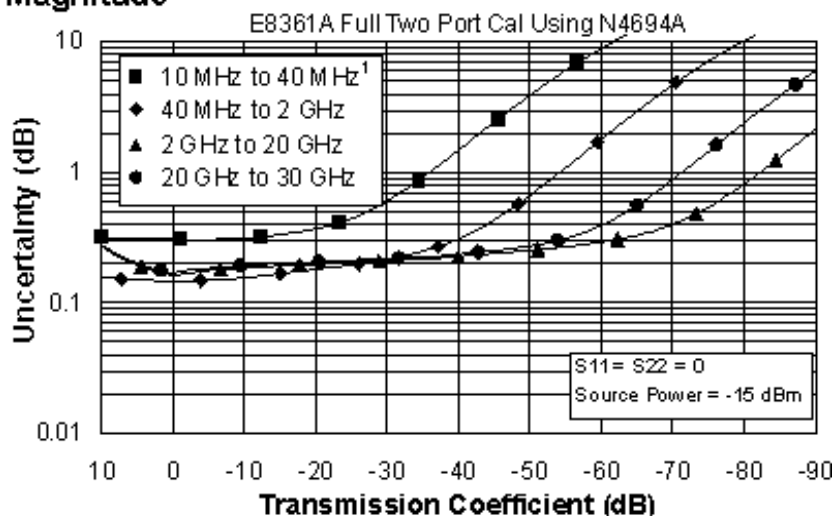


## Magnitude

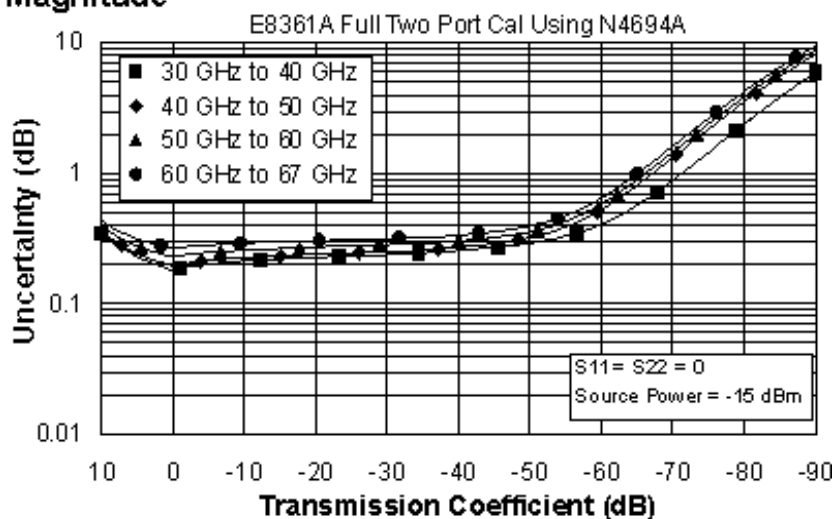


1 Typical performance.

## Phase

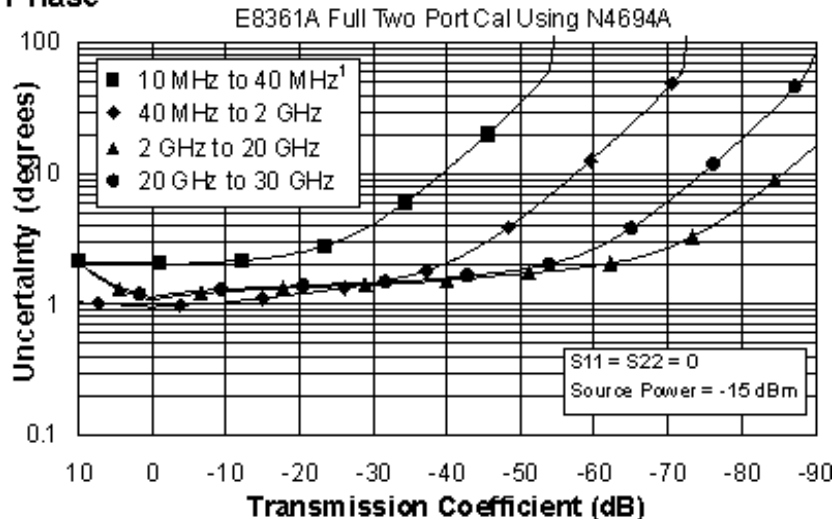


## Phase

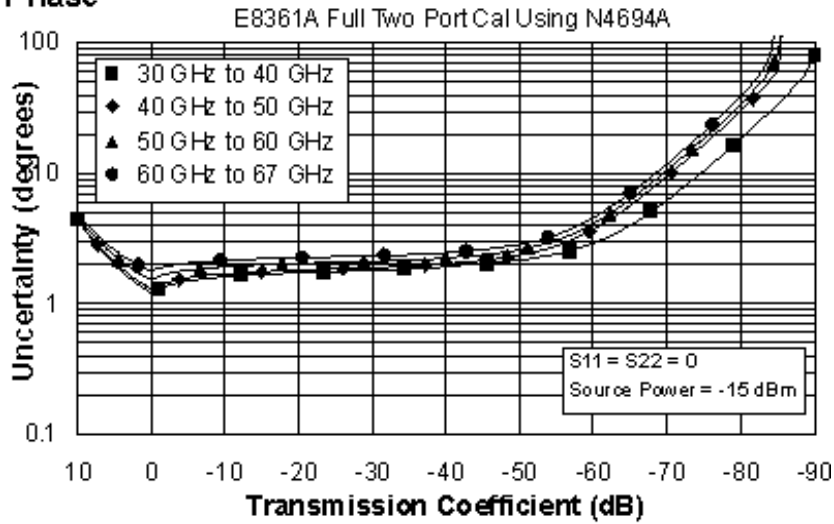


1 Typical performance.

## Reflection Uncertainty (Specifications)

### Magnitude

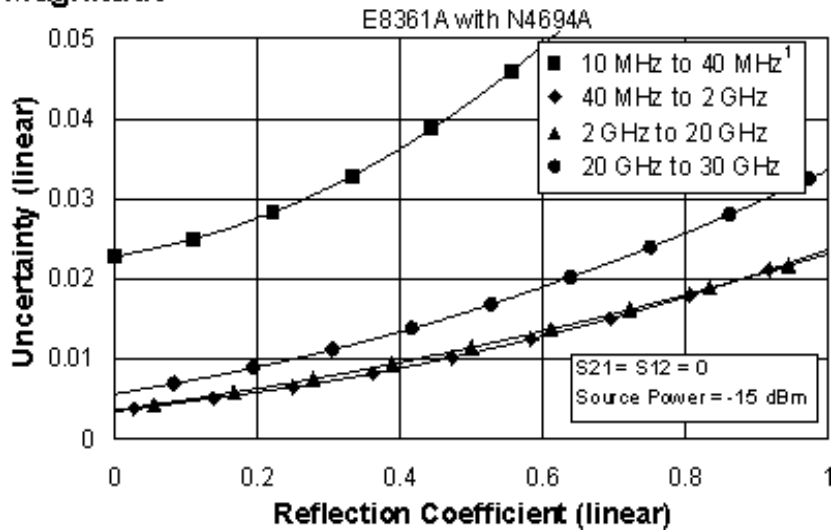


## Magnitude

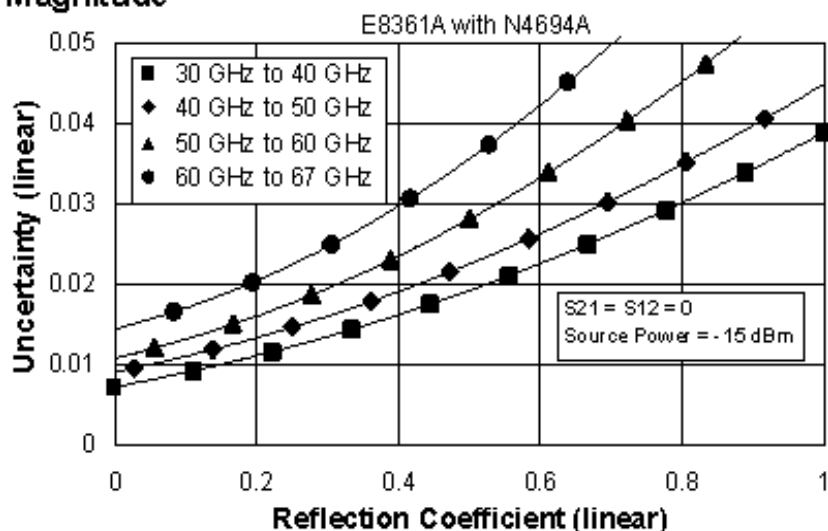


1 Typical performance.

## Phase

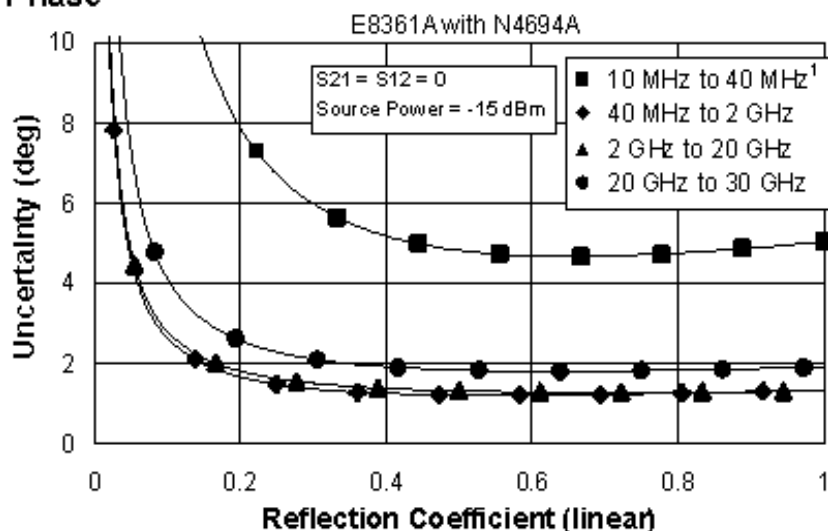

## Phase

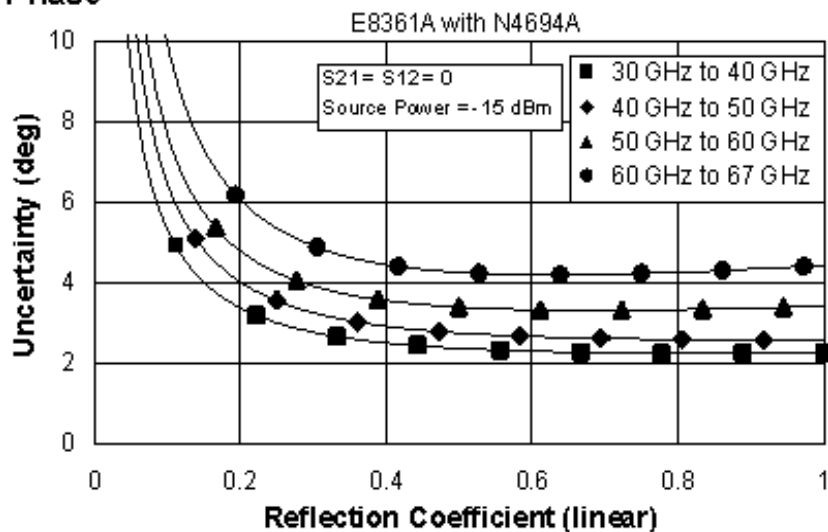

1 Typical performance.

**Table 5. N4694A Calibration Kit****E8361A - Fully Optioned (Option 014, UNL, 016, 080, and 081)**

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E8361A analyzers, N4694A (1.85mm) ECal module, N4697F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB)        |                    |                    |                    |
|-----------------------|---------------------------|--------------------|--------------------|--------------------|
|                       | 10 to 40 MHz <sup>1</sup> | 40 MHz to 2 GHz    | 2 to 20 GHz        | 20 to 30 GHz       |
| Directivity           | 33                        | 50                 | 50                 | 46                 |
| Source Match          | 25                        | 38                 | 39                 | 35                 |
| Load Match            | 30                        | 39                 | 39                 | 38                 |
| Reflection Tracking   | ±0.050<br>+0.02/°C        | ±0.040<br>+0.02/°C | ±0.040<br>+0.02/°C | ±0.050<br>+0.03/°C |
| Transmission Tracking | ±0.260<br>+0.02/°C        | ±0.121<br>+0.02/°C | ±0.139<br>+0.02/°C | ±0.138<br>+0.03/°C |

<sup>1</sup> Typical performance.


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 30 to 40 GHz       | 40 to 50 GHz       | 50 to 60 GHz       | 60 to 67 GHz       |
| Directivity           | 44                 | 42                 | 41                 | 38                 |
| Source Match          | 25                 | 38                 | 39                 | 35                 |
| Load Match            | 30                 | 39                 | 39                 | 38                 |
| Reflection Tracking   | ±0.050<br>+0.02/°C | ±0.040<br>+0.02/°C | ±0.040<br>+0.02/°C | ±0.050<br>+0.03/°C |
| Transmission Tracking | ±0.260<br>+0.02/°C | ±0.121<br>+0.02/°C | ±0.139<br>+0.02/°C | ±0.138<br>+0.03/°C |

### Transmission Uncertainty (Specifications)

## Magnitude

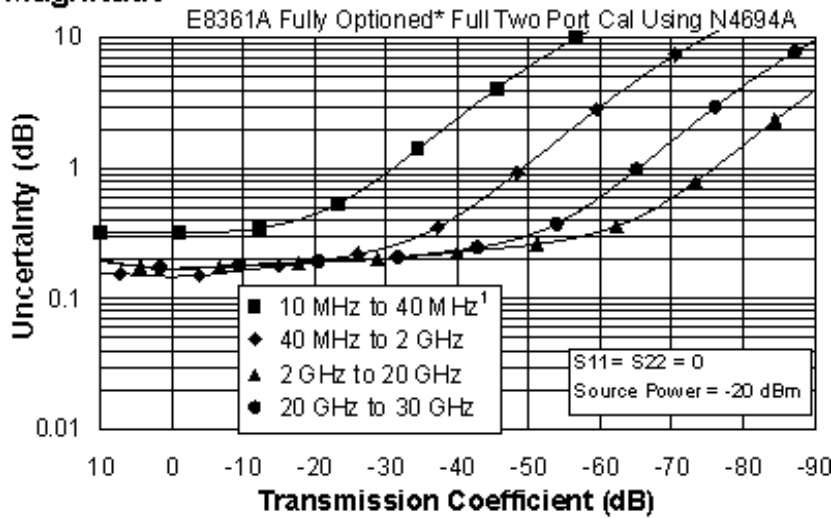


## Magnitude

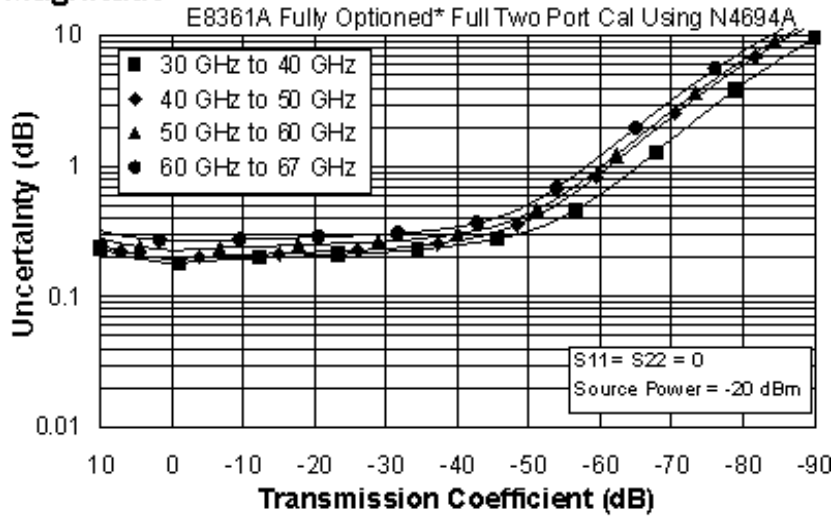


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)

1 Typical performance.

## Phase

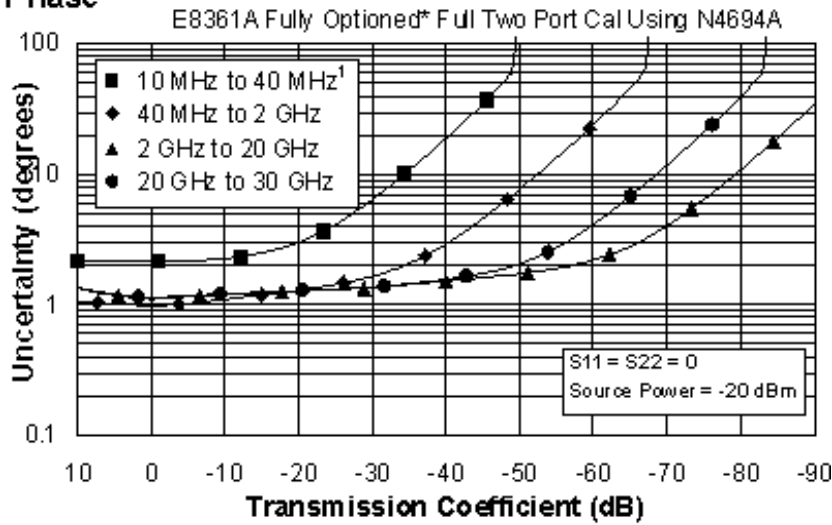

## Phase

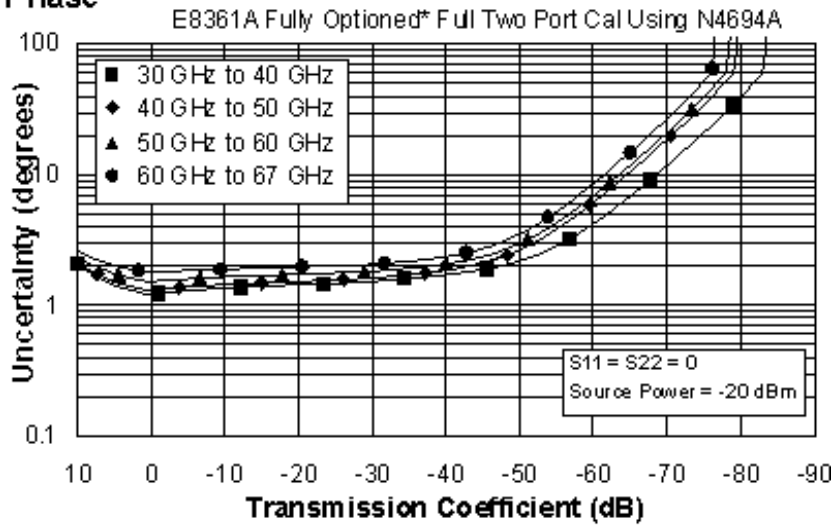


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)

<sup>1</sup> Typical performance.


## Reflection Uncertainty (Specifications)



## Magnitude

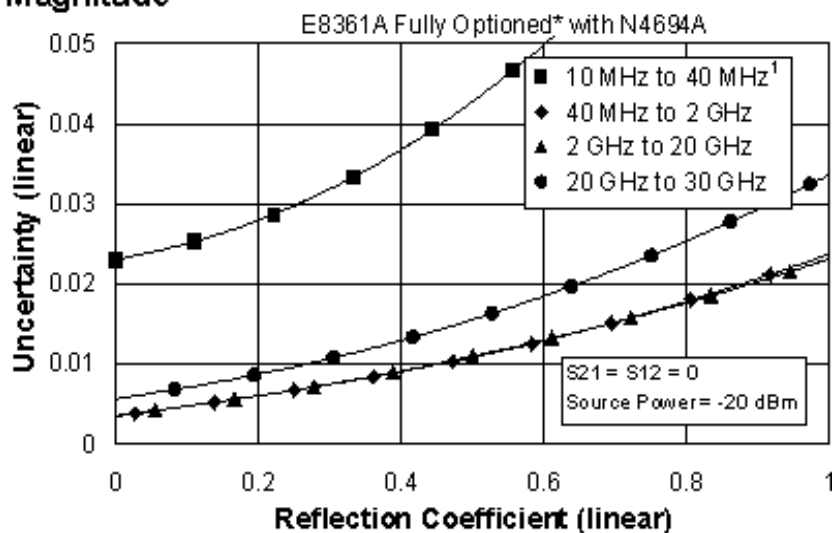


## Magnitude

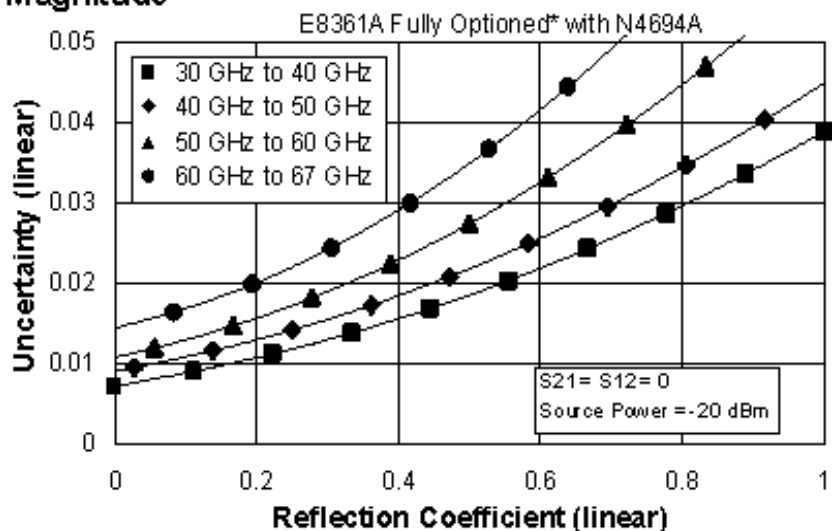


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)

1 Typical performance.

## Phase

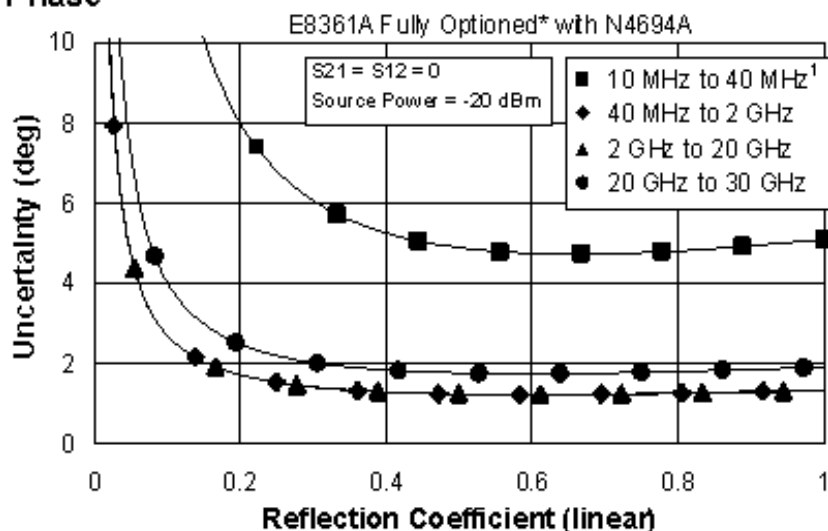

## Phase

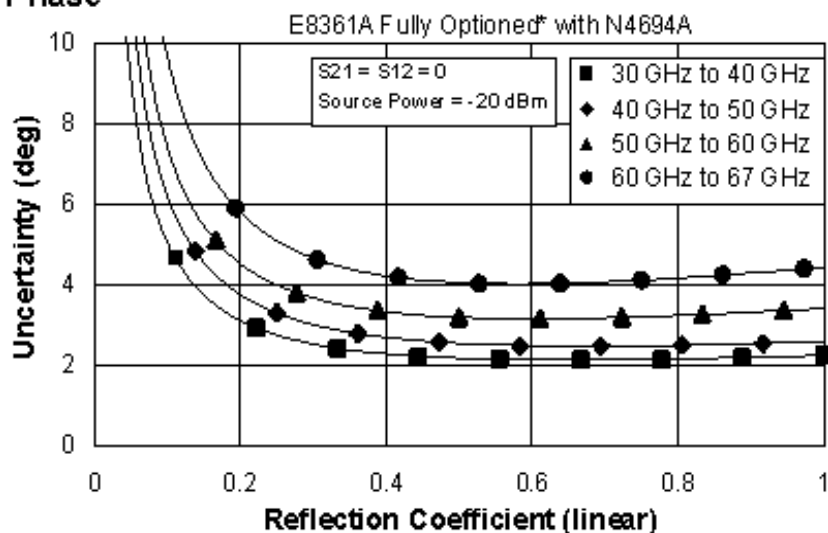

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (Option 014, UNL, 016, 080, and 081)

<sup>1</sup> Typical performance.

This document does not present specifications for the 85058E Calibration Kit. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the data and curves for the 85058E Calibration Kit or your PNA setup. View the [equations](#) used to generate the uncertainty curve.

## E8363/4B Corrected System Performance with 2.4mm Connectors

---

### 85056A Calibration Kit:

Standard Configuration and Standard Power Range (E8363/4B)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

### 85056D Calibration Kit:

Standard Configuration and Standard Power Range (E8363/4B)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

---


**Table 3.** 85056A Calibration Kit  
Standard Configuration and Standard Power Range  
(E8363/4B)

Applies to the E8363/4B analyzers, 85056A (2.4mm) calibration kit, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 45 MHz to<br>2 GHz                      | 2 to<br>20 GHz                          | 20 to<br>40 GHz                         | 40 to<br>50 GHz                         |
| Directivity           | 42                                      | 42                                      | 38                                      | 36                                      |
| Source Match          | 41                                      | 38                                      | 33                                      | 31                                      |
| Load Match            | 42                                      | 42                                      | 37                                      | 35                                      |
| Reflection Tracking   | $\pm 0.001$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.008$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.020$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.027$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.010$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.049$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.105$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.170$<br>$+0.03/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications)

### Magnitude

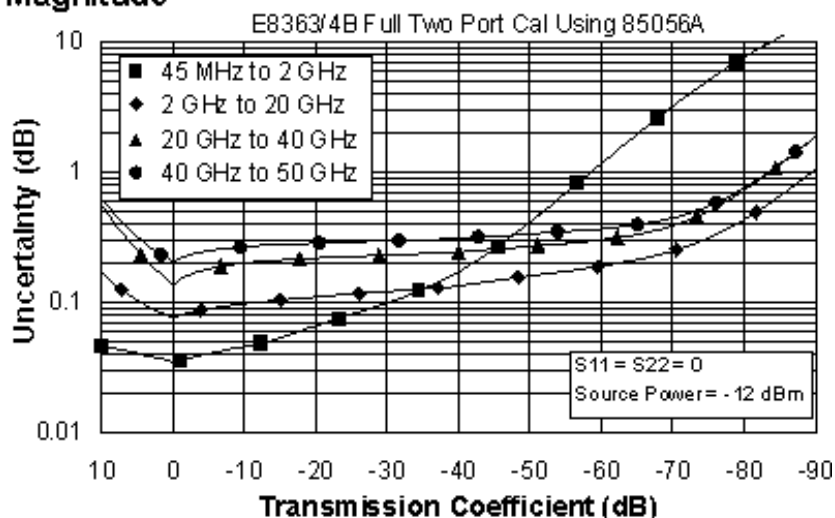



### Phase

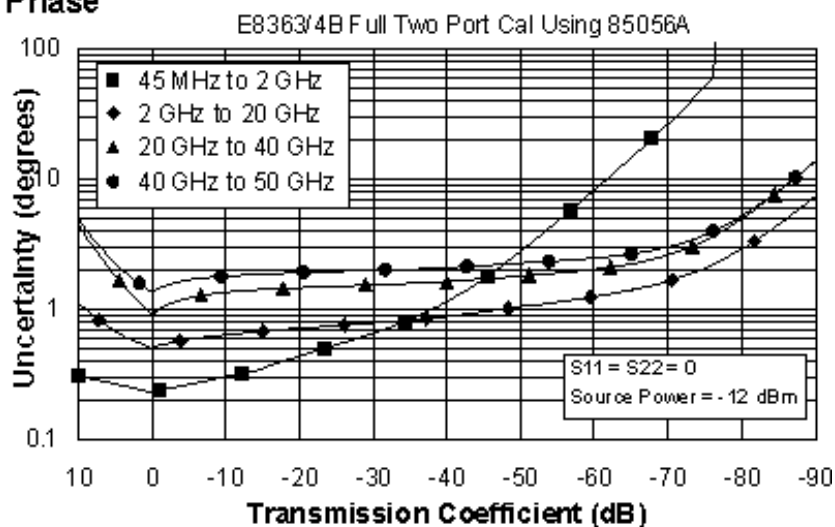

### Reflection Uncertainty (Specifications)

#### Magnitude

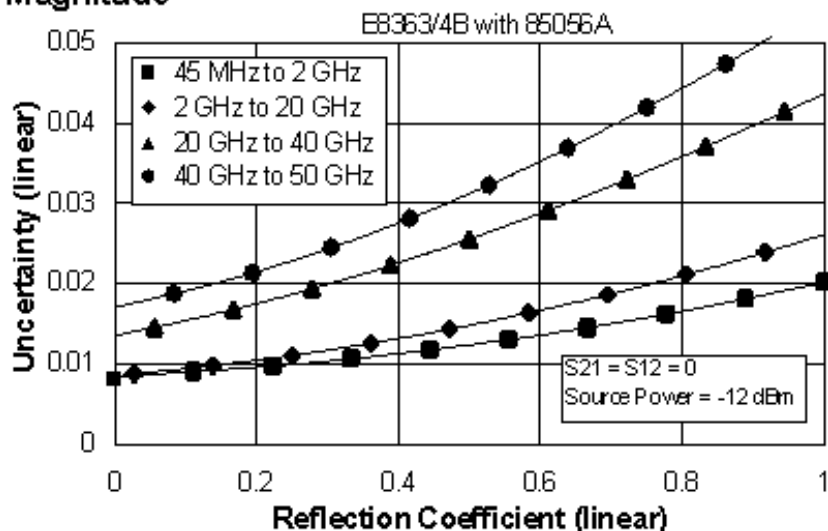

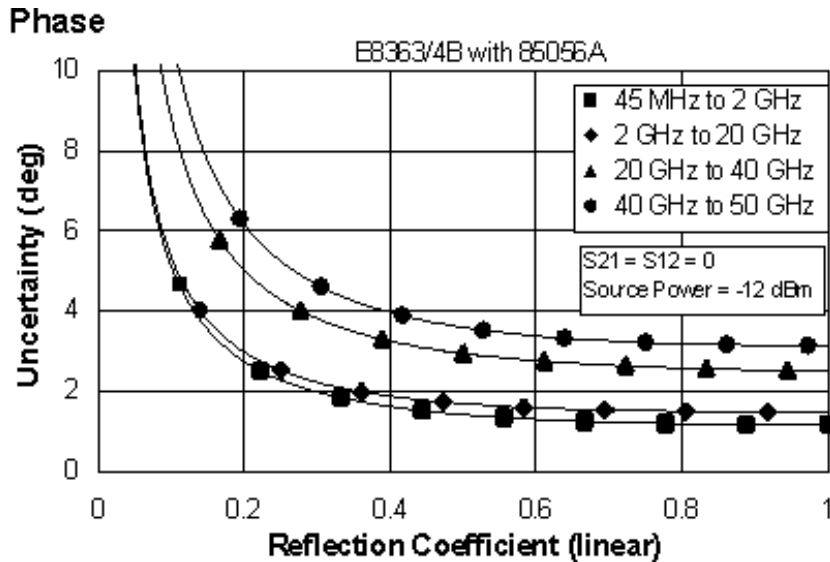

**Table 4.** 85056A Calibration Kit  
Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E8363/4B analyzers, 85056A (2.4mm) calibration kit, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to<br>2 GHz | 2 to<br>20 GHz     | 20 to<br>40 GHz    | 40 to<br>50 GHz    |
| Directivity           | 42                 | 42                 | 38                 | 36                 |
| Source Match          | 41                 | 38                 | 33                 | 31                 |
| Load Match            | 42                 | 42                 | 37                 | 35                 |
| Reflection Tracking   | ±0.001<br>+0.02/°C | ±0.008<br>+0.02/°C | ±0.020<br>+0.02/°C | ±0.027<br>+0.03/°C |
| Transmission Tracking | ±0.019<br>+0.02/°C | ±0.053<br>+0.02/°C | ±0.109<br>+0.02/°C | ±0.182<br>+0.03/°C |

**Transmission Uncertainty (Specifications)**


## Magnitude

E8363/4B Fully Optioned\* Full Two Port Cal Using 85056A

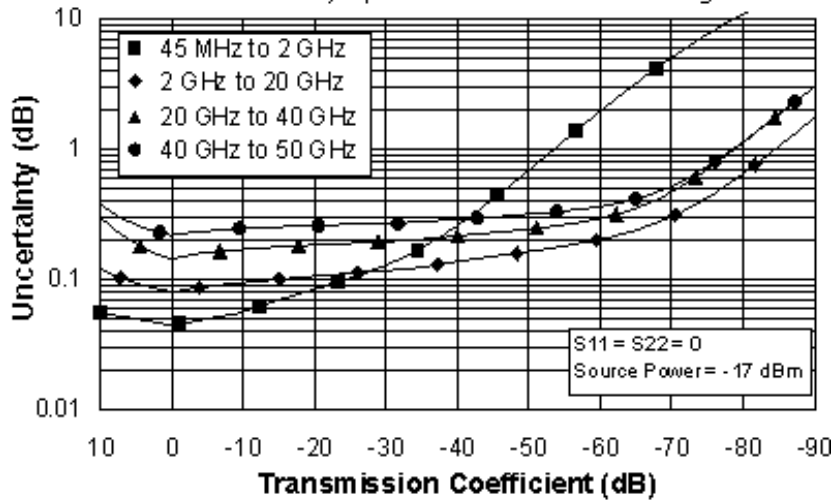

## Phase


E8363/4B Fully Optioned\* Full Two Port Cal Using 85056A

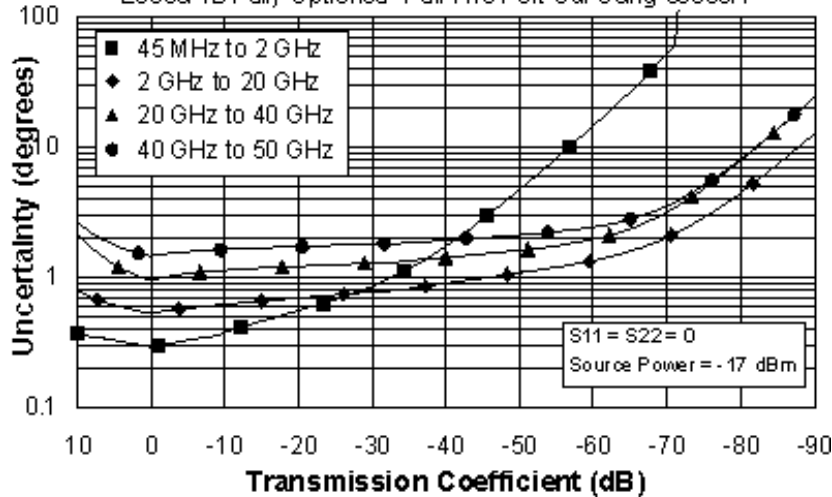


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

## Magnitude

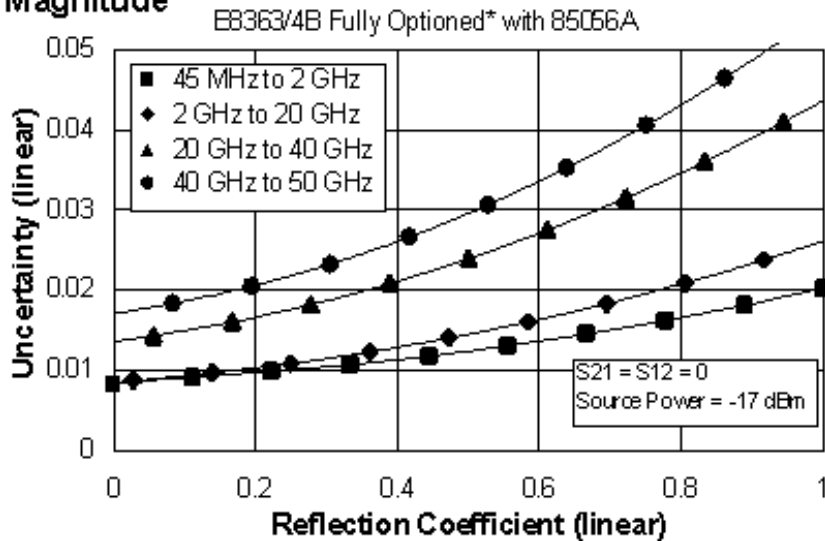

## Phase

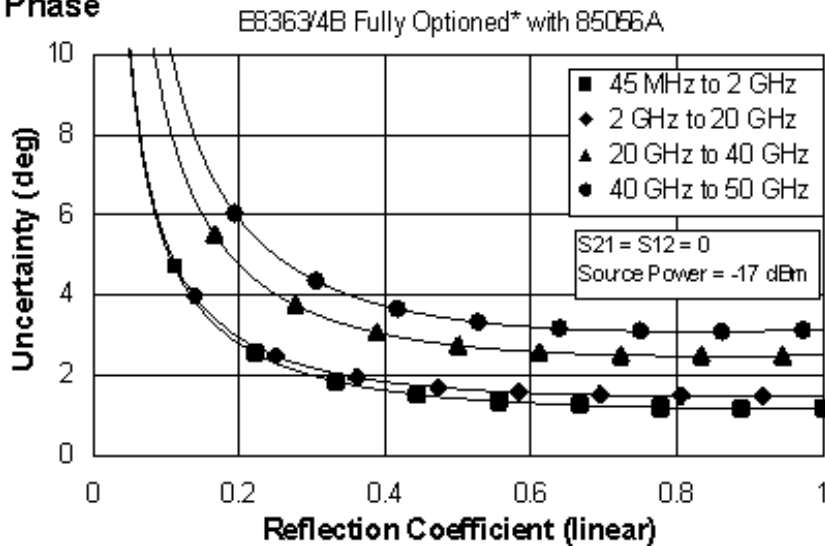

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)


**Table 5.** 85056D Calibration Kit

Standard Configuration and Standard Power Range  
 (E8363/4B)


Applies to the, E8363/4B analyzers, 85056D (2.4mm) calibration kit, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |                                         |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 45 MHz to 2 GHz                         | 2 to 20 GHz                             | 20 to 40 GHz                            | 40 to 50 GHz                            |
| Directivity           | 42                                      | 34                                      | 26                                      | 26                                      |
| Source Match          | 40                                      | 30                                      | 24                                      | 23                                      |
| Load Match            | 42                                      | 33                                      | 25                                      | 25                                      |
| Reflection Tracking   | $\pm 0.002$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.029$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.079$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.075$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.011$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.121$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.347$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.462$<br>$+0.03/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications) Magnitude

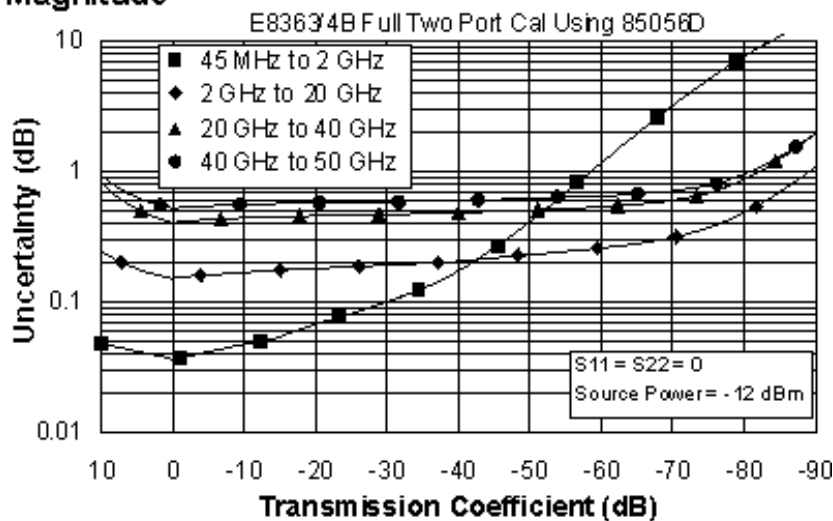


### Phase

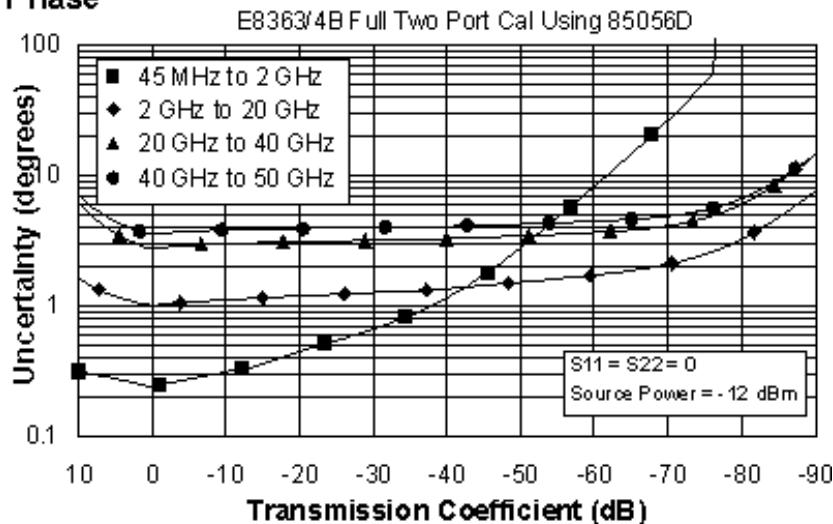




## Reflection Uncertainty (Specifications) Magnitude

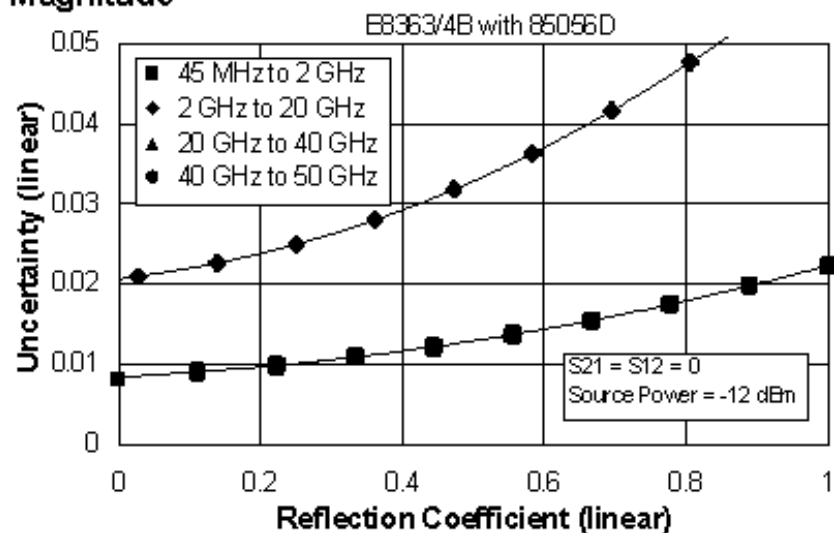

## Phase

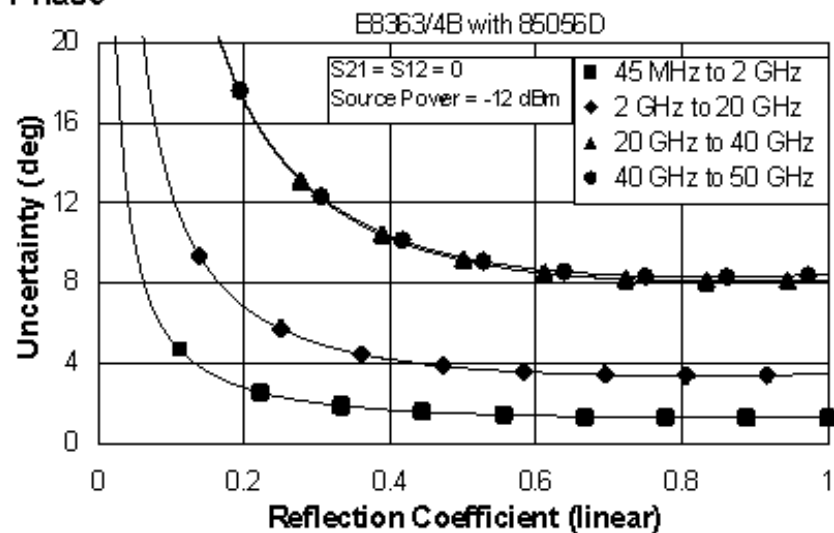

**Table 6.** 85056D Calibration Kit

Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E8363/4B analyzers, 85056D (2.4mm) calibration kit, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)      |                         |                         |                         |
|-----------------------|-------------------------|-------------------------|-------------------------|-------------------------|
|                       | 45 MHz to<br>2 GHz      | 2 to<br>20 GHz          | 20 to<br>40 GHz         | 40 to<br>50 GHz         |
| Directivity           | 42                      | 34                      | 26                      | 26                      |
| Source Match          | 40                      | 30                      | 24                      | 23                      |
| Load Match            | 42                      | 33                      | 25                      | 25                      |
| Reflection Tracking   | $\pm 0.002$<br>+0.02/°C | $\pm 0.029$<br>+0.02/°C | $\pm 0.079$<br>+0.02/°C | $\pm 0.075$<br>+0.03/°C |
| Transmission Tracking | $\pm 0.022$<br>+0.02/°C | $\pm 0.130$<br>+0.02/°C | $\pm 0.365$<br>+0.02/°C | $\pm 0.498$<br>+0.03/°C |

### Transmission Uncertainty (Specifications)

#### Magnitude

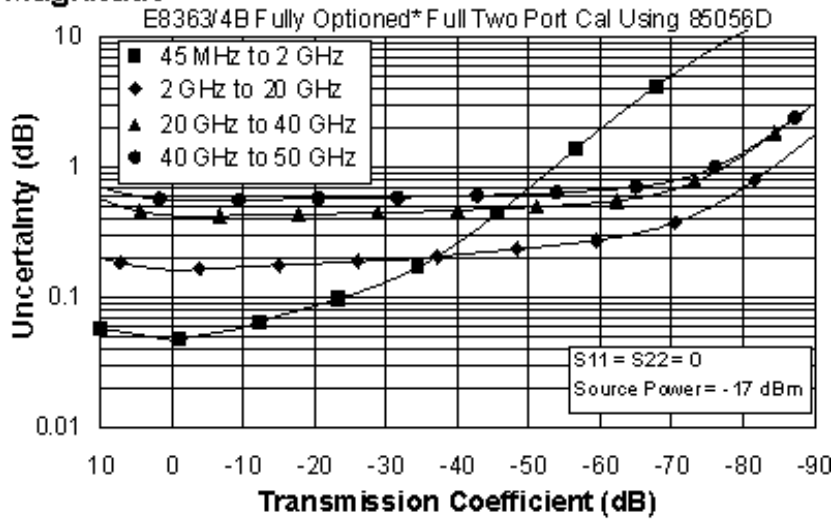


## Phase

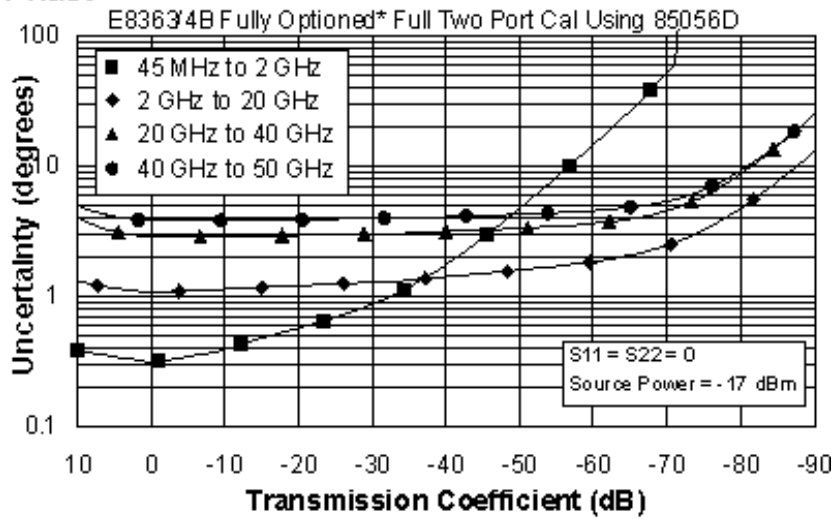


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

### Magnitude

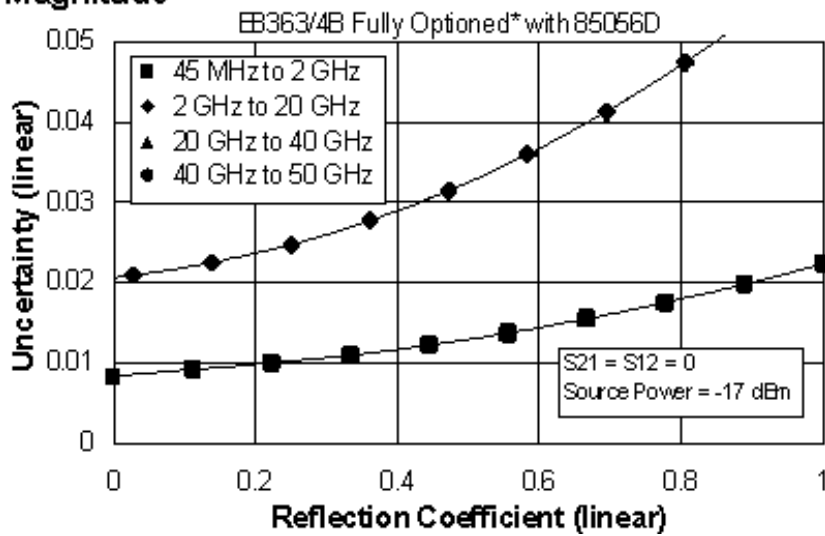

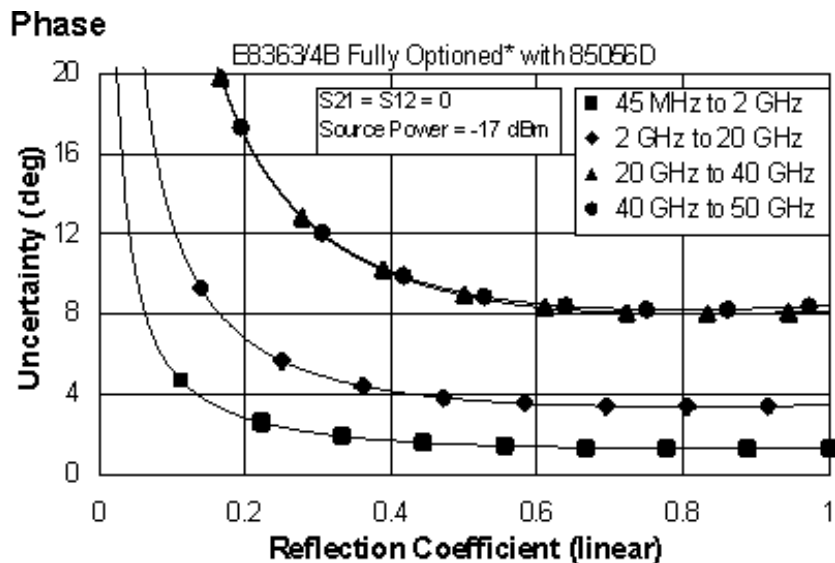

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## E8361A Corrected System Performance with 2.4mm Connectors

---

### 85056A Calibration Kit:

**Standard Configuration and Standard Power Range (E8361A)**

**Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)**

### N4693A Electronic Calibration Module

**Standard Configuration and Standard Power Range (E8361A)**

**Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)**

---

**Table 6.** 85056A Calibration Kit  
E8361A - Standard Configuration and Standard Power Range


Applies to the E8361A analyzers, 85056A (2.4mm) Calibration Kit, 85133F flexible test port cable set, and a full 2-port calibration. (2.4 mm connectors are mateable with 1.85 mm connectors.) Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to<br>2 GHz | 2 to<br>20 GHz     | 20 to<br>40 GHz    | 40 to<br>50 GHz    |
| Directivity           | 42                 | 42                 | 38                 | 36                 |
| Source Match          | 41                 | 38                 | 33                 | 31                 |
| Load Match            | 42                 | 42                 | 37                 | 35                 |
| Reflection Tracking   | ±0.001<br>+0.02/°C | ±0.008<br>+0.02/°C | ±0.020<br>+0.02/°C | ±0.027<br>+0.03/°C |
| Transmission Tracking | ±0.035<br>+0.02/°C | ±0.060<br>+0.02/°C | ±0.146<br>+0.02/°C | ±0.181<br>+0.03/°C |

### Transmission Uncertainty (Specifications)

## Magnitude

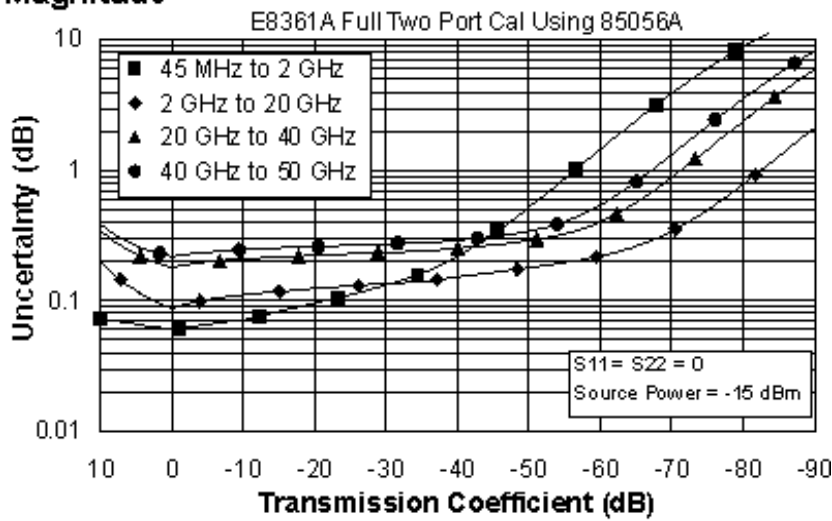


## Phase

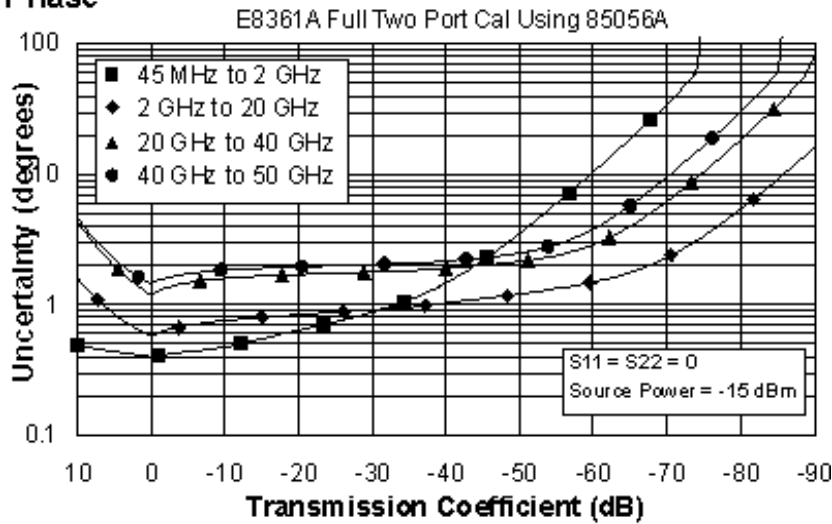


## Reflection Uncertainty (Specifications)

### Magnitude

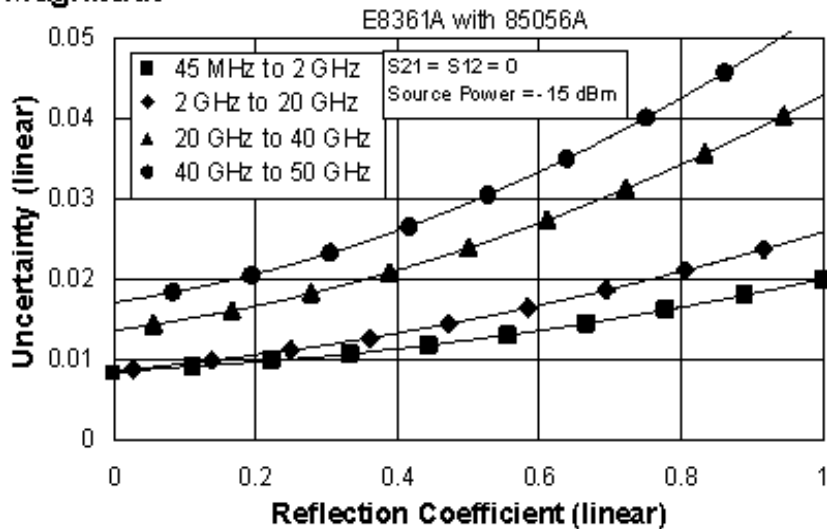

## Phase

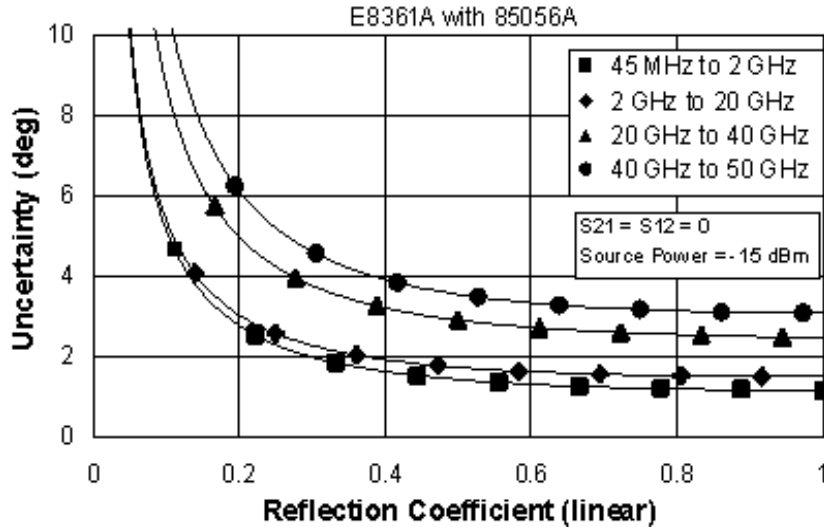

**Table 7.** 85056A Calibration Kit

E8361A - Fully Optioned (Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E8361A analyzers, 85056A (2.4mm) Calibration Kit, 85133F flexible test port cable set, and a full 2-port calibration. (2.4 mm connectors are mateable with 1.85 mm connectors.) Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to<br>2 GHz | 2 to<br>20 GHz     | 20 to<br>40 GHz    | 40 to<br>50 GHz    |
| Directivity           | 42                 | 42                 | 38                 | 36                 |
| Source Match          | 41                 | 38                 | 33                 | 31                 |
| Load Match            | 42                 | 41                 | 37                 | 35                 |
| Reflection Tracking   | ±0.001<br>+0.02/°C | ±0.008<br>+0.02/°C | ±0.020<br>+0.02/°C | ±0.027<br>+0.03/°C |
| Transmission Tracking | ±0.040<br>+0.02/°C | ±0.086<br>+0.02/°C | ±0.123<br>+0.02/°C | ±0.155<br>+0.03/°C |

## Transmission Uncertainty (Specifications)

## Magnitude

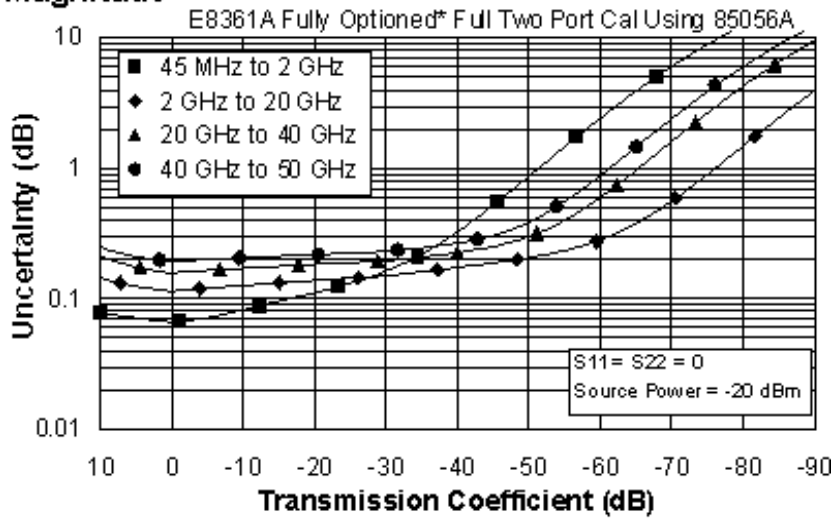

## Phase

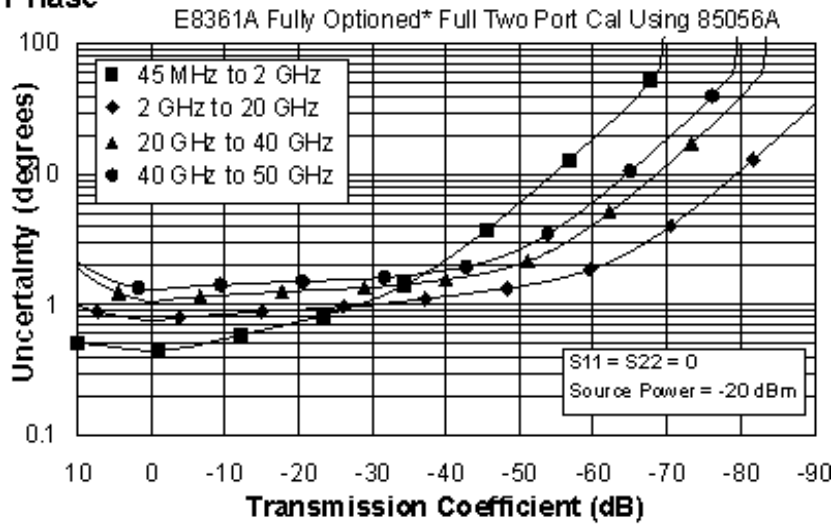


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)


## Reflection Uncertainty (Specifications)



## Magnitude

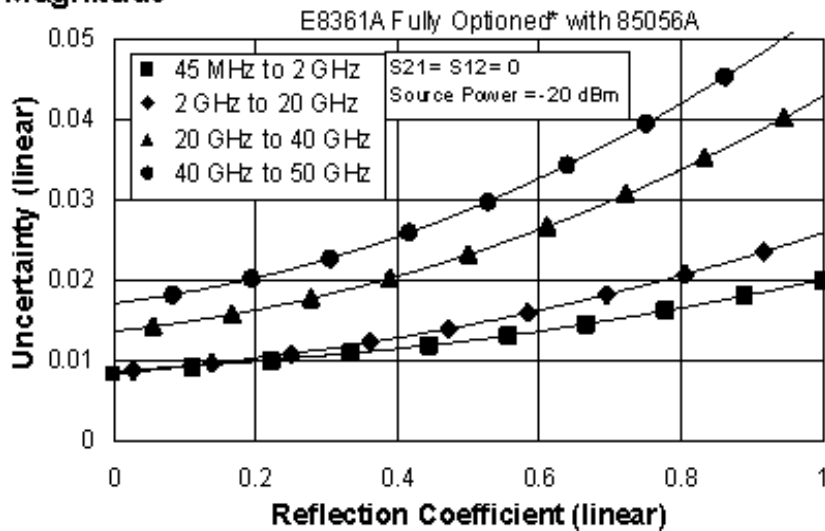

## Phase

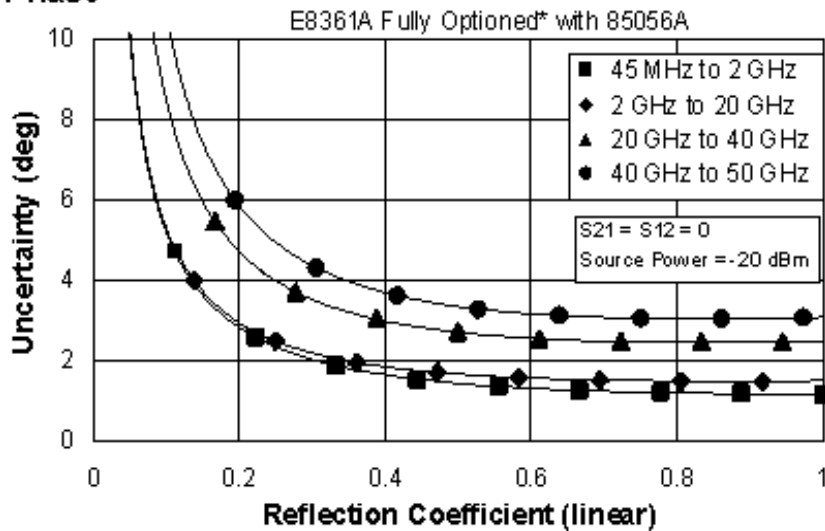

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)

**Table 8.** N4693A Electronic Calibration Module

E8361A - Standard Configuration and Standard Power Range


Applies to the, E8361A analyzers, N4693A (2.4mm) Electronic Calibration Module, 85133F flexible test port cable set, and a full 2-port calibration. (2.4 mm connectors are mateable with 1.85 mm connectors.) Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                    |                                       |                                       |                                       |
|-----------------------|---------------------------------------|---------------------------------------|---------------------------------------|---------------------------------------|
|                       | 45 MHz to<br>2 GHz                    | 2 to<br>20 GHz                        | 20 to<br>40 GHz                       | 40 to<br>50 GHz                       |
| Directivity           | 55                                    | 49                                    | 43                                    | 41                                    |
| Source Match          | 46                                    | 42                                    | 35                                    | 30                                    |
| Load Match            | 43                                    | 41                                    | 37                                    | 36                                    |
| Reflection Tracking   | $\pm 0.030$<br>$+0.02/^\circ\text{C}$ | $\pm 0.040$<br>$+0.02/^\circ\text{C}$ | $\pm 0.060$<br>$+0.02/^\circ\text{C}$ | $\pm 0.080$<br>$+0.03/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.059$<br>$+0.02/^\circ\text{C}$ | $\pm 0.079$<br>$+0.02/^\circ\text{C}$ | $\pm 0.110$<br>$+0.02/^\circ\text{C}$ | $\pm 0.125$<br>$+0.03/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

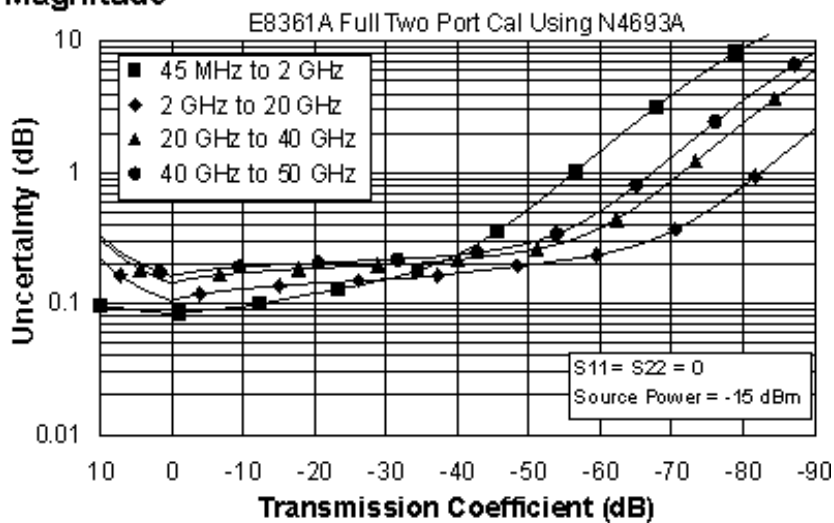


### Phase

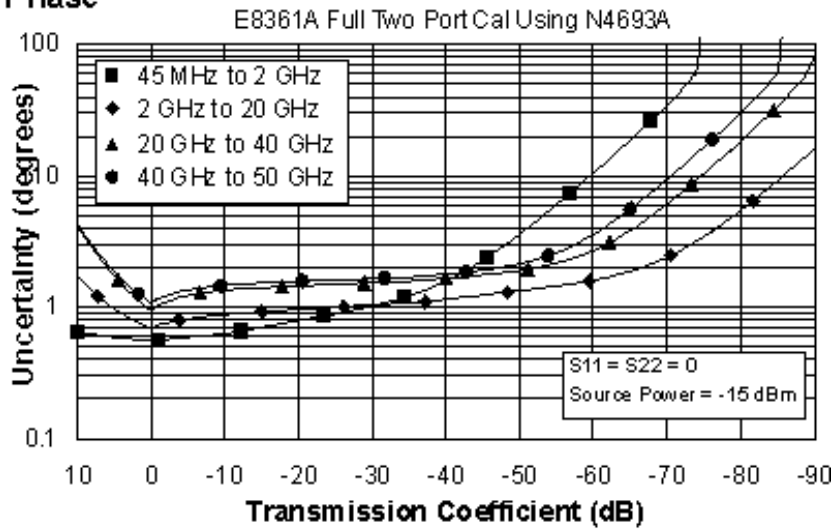


### Reflection Uncertainty (Specifications)

#### Magnitude

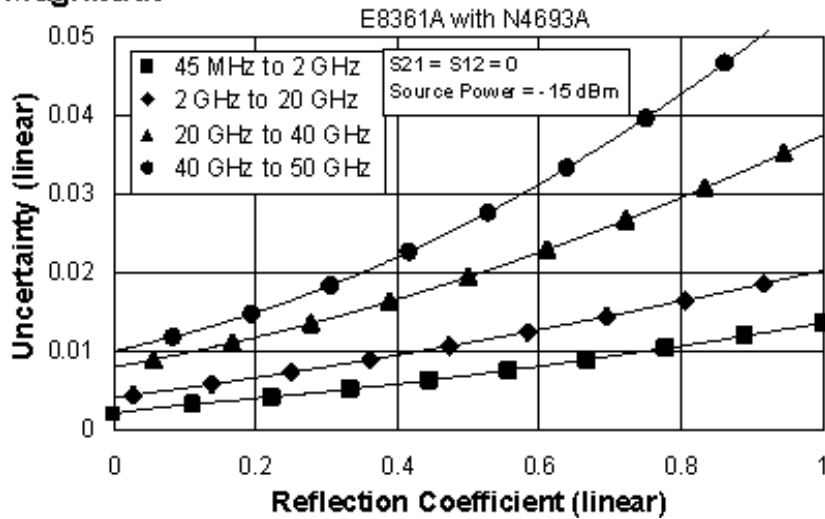

#### Phase

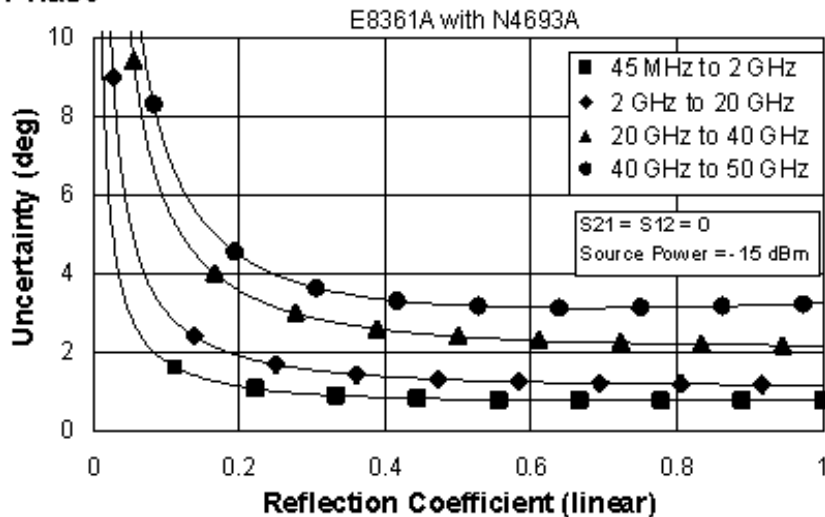

**Table 9. N4693A Electronic Calibration Module**  
**E8361A - Fully Optioned (Option 014, UNL, 016, 080, and 081)**

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E8361A analyzers, N4693A(2.4mm) Electronic Calibration Module, 85133F flexible test port cable set, and a full 2-port calibration. (2.4 mm connectors are mateable with 1.85 mm connectors.) Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to 2 GHz    | 2 to 20 GHz        | 20 to 40 GHz       | 40 to 50 GHz       |
| Directivity           | 55                 | 49                 | 43                 | 41                 |
| Source Match          | 46                 | 42                 | 35                 | 30                 |
| Load Match            | 43                 | 41                 | 37                 | 36                 |
| Reflection Tracking   | ±0.030<br>+0.02/°C | ±0.040<br>+0.02/°C | ±0.060<br>+0.02/°C | ±0.080<br>+0.03/°C |
| Transmission Tracking | ±0.060<br>+0.02/°C | ±0.082<br>+0.02/°C | ±0.106<br>+0.02/°C | ±0.121<br>+0.03/°C |

**Transmission Uncertainty (Specifications)**

**Magnitude**

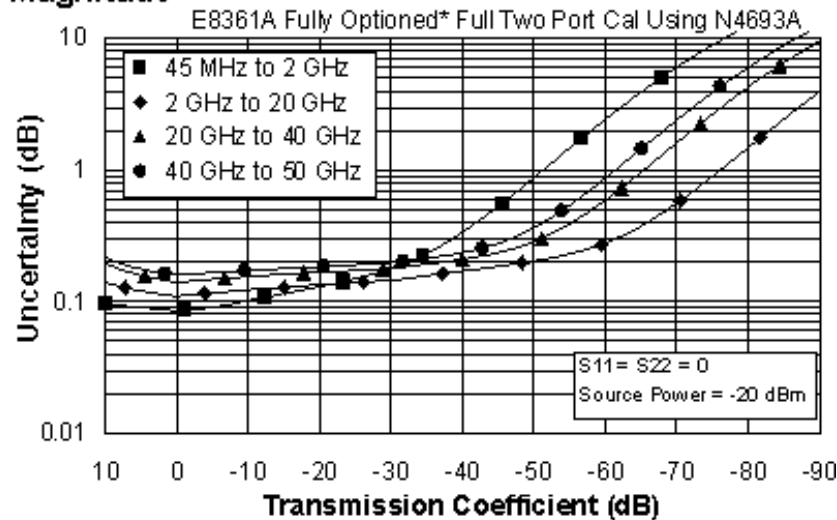


## Phase

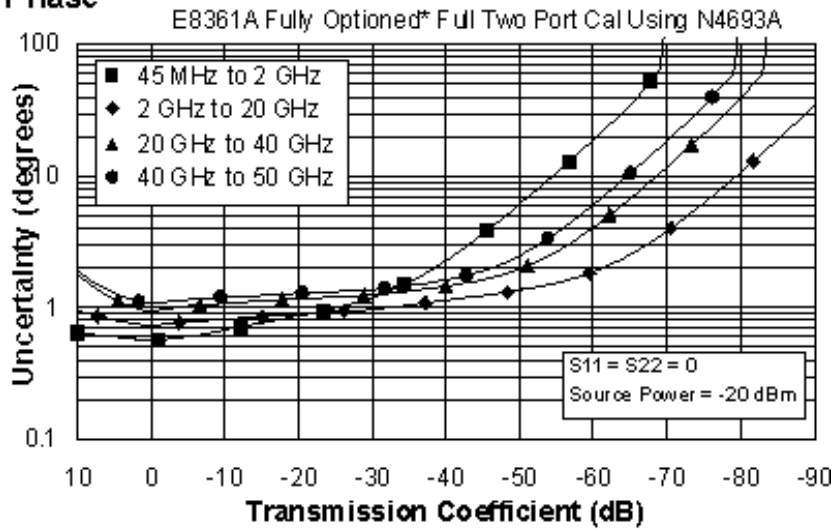


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

### Magnitude

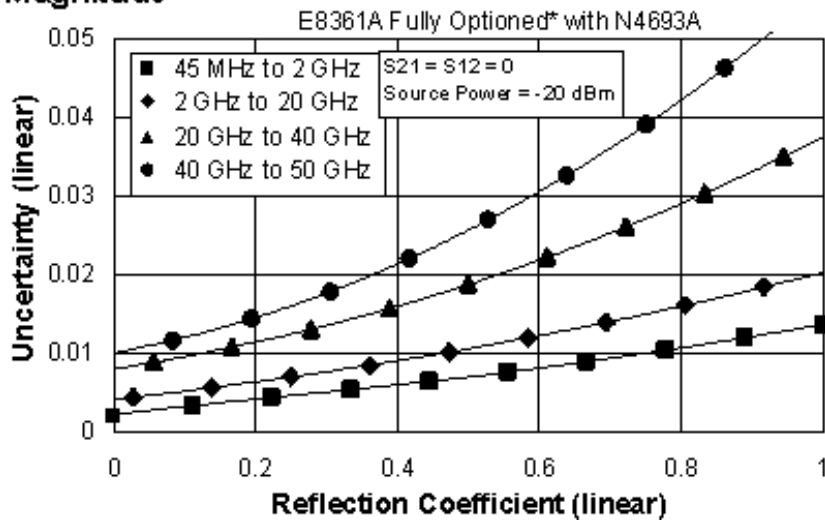

# Phase

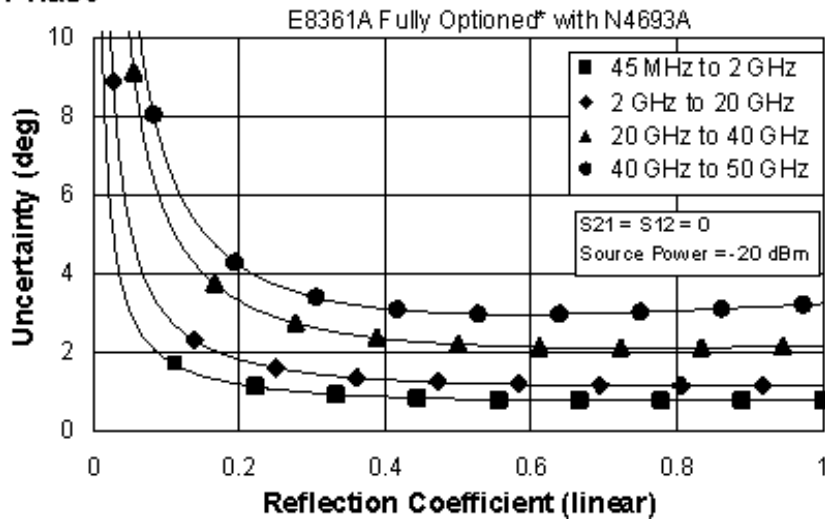

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E8361A - Option 014, UNL, 016, 080, and 081)

This document does not present specifications for the 85056D or 85056K Calibration Kit. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the data and curves for the 85056D or 85056K Calibration Kit or your PNA setup. View the [equations](#) used to generate the uncertainty curve

## N5230A Corrected System Performance with 2.4mm Connectors

Options 220/225, 420/425, and 520/525

---

### 85056A Calibration Kit:

[N5230A - Option 420 or 520 \(Standard Test Set and Standard Power Range\)](#)

[N5230A Option 425 or 525  
Configurable Test Set and Extended Power Range](#)

### N4693A Electronic Calibration Module

[N5230A - Option 420 or 520  
Standard Test Set and Standard Power Range](#)

[N5230A Option 425 or 525  
Configurable Test Set and Extended Power Range](#)

---

### Table 9. 85056A Calibration Kit

#### N5230A - Option 420 or 520 (Standard Test Set and Standard Power Range)


Applies to the N5230A Option 420 or 520 analyzers, 85056A (2.4mm) Electronic Calibration Module, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to<br>2 GHz | 2 to<br>20 GHz     | 20 to<br>40 GHz    | 40 to<br>50 GHz    |
| Directivity           | 42                 | 42                 | 38                 | 36                 |
| Source Match          | 41                 | 38                 | 33                 | 31                 |
| Load Match            | 42                 | 42                 | 37                 | 35                 |
| Reflection Tracking   | ±0.001<br>+0.02/°C | ±0.008<br>+0.02/°C | ±0.020<br>+0.02/°C | ±0.027<br>+0.03/°C |
| Transmission Tracking | ±0.019<br>+0.02/°C | ±0.060<br>+0.02/°C | ±0.129<br>+0.02/°C | ±0.211<br>+0.03/°C |

### Transmission Uncertainty (Specifications)

## Magnitude

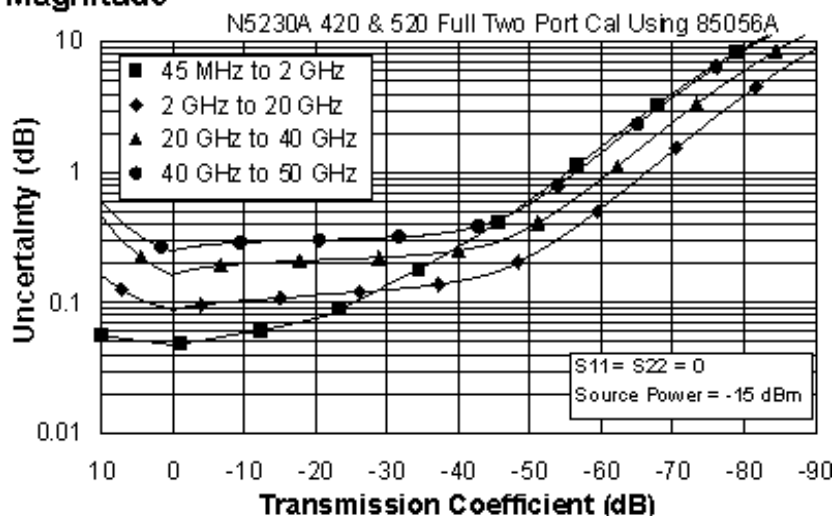


## Phase

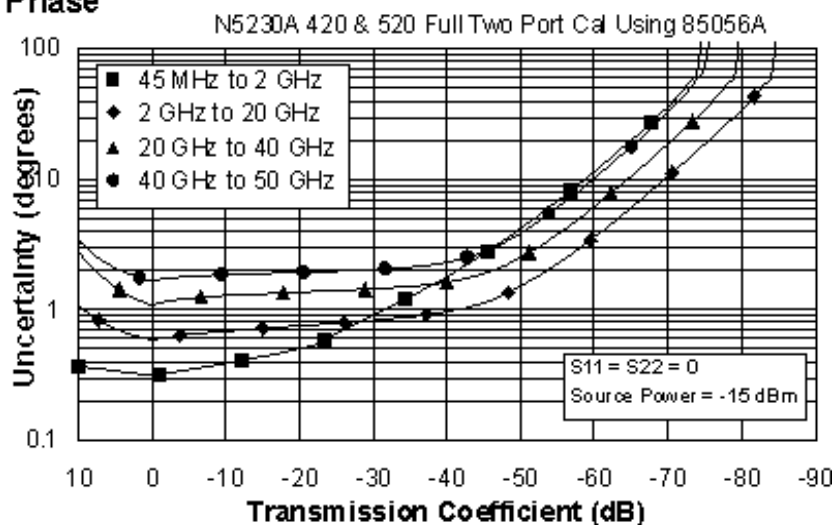


## Reflection Uncertainty (Specifications)

### Magnitude

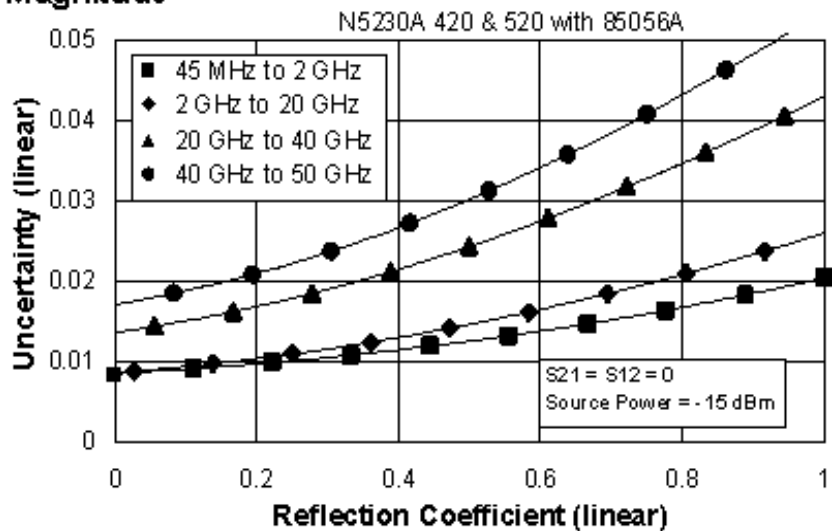



## Phase

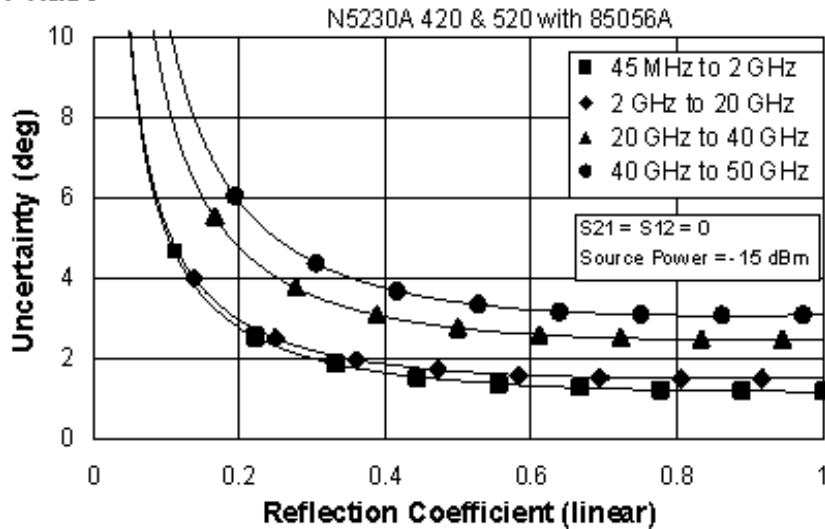

**Table 10.** 85056A Calibration Kit

N5230A - Option 425 or 525 (Configurable Test Set and Extended Power Range)


Applies to the N5230A Option 425 or 525 analyzers, 85056A (2.4mm) Electronic Calibration Module, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 45 MHz to<br>2 GHz                      | 2 to<br>20 GHz                          | 20 to<br>40 GHz                         | 40 to<br>50 GHz                         |
| Directivity           | 42                                      | 42                                      | 38                                      | 36                                      |
| Source Match          | 41                                      | 38                                      | 33                                      | 31                                      |
| Load Match            | 42                                      | 42                                      | 37                                      | 35                                      |
| Reflection Tracking   | $\pm 0.001$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.008$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.020$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.027$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.019$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.057$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.124$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.211$<br>$+0.03/^{\circ}\text{C}$ |

## Transmission Uncertainty (Specifications)

## Magnitude

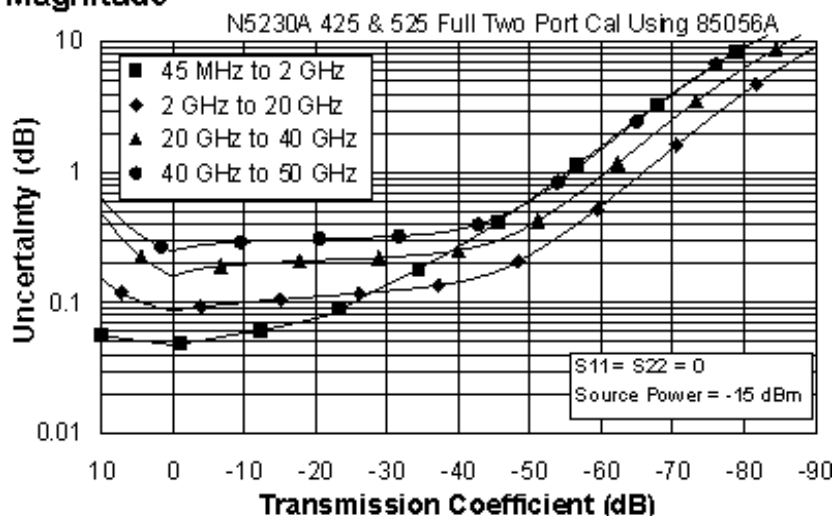


## Phase

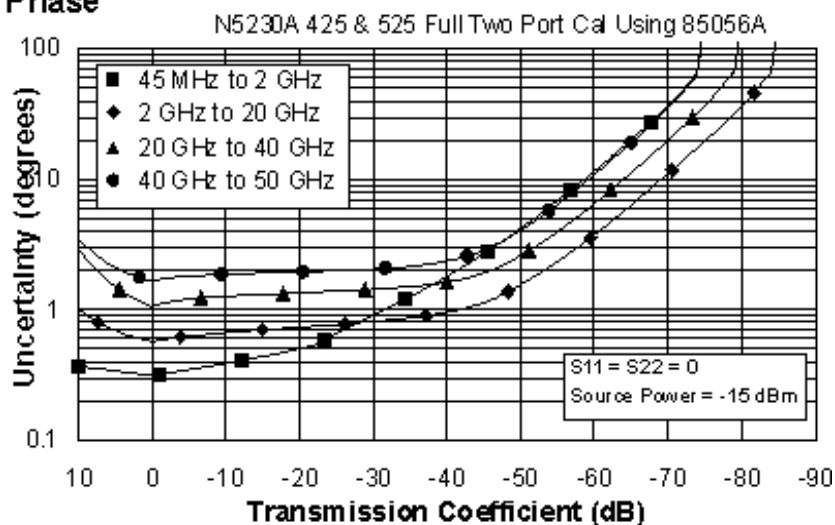


## Reflection Uncertainty (Specifications)

### Magnitude

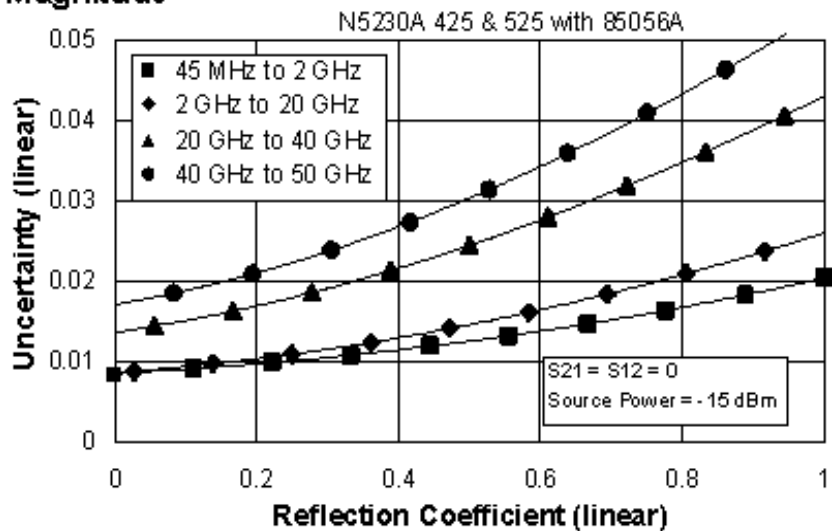

## Phase

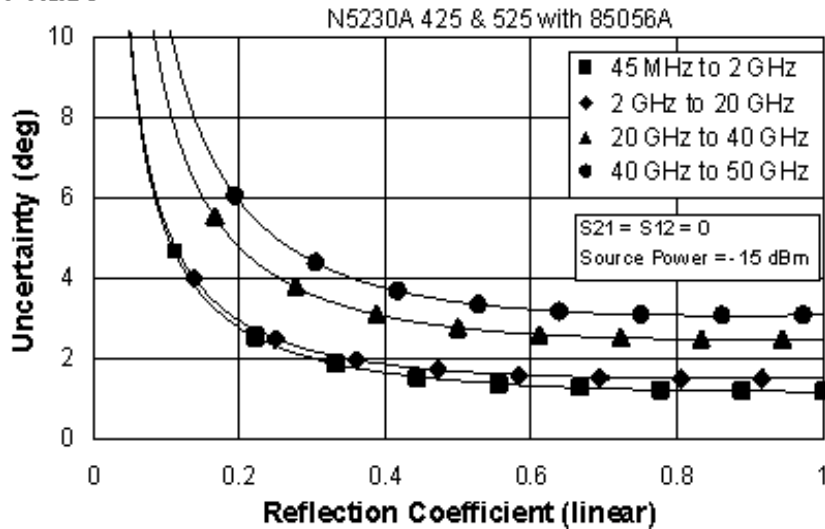

**Table 11. N4693A Electronic Calibration Module**  
 N5230A - Option 420 or 520 (Standard Test Set and Standard Power Range)


Applies to the N5230A Option 420 or 520 analyzers, N4693A (2.4mm) Electronic Calibration Module, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 45 MHz to<br>2 GHz                      | 2 to<br>20 GHz                          | 20 to<br>40 GHz                         | 40 to<br>50 GHz                         |
| Directivity           | 55                                      | 49                                      | 43                                      | 41                                      |
| Source Match          | 46                                      | 42                                      | 35                                      | 30                                      |
| Load Match            | 43                                      | 41                                      | 37                                      | 36                                      |
| Reflection Tracking   | $\pm 0.030$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.040$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.060$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.080$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.056$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.079$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.107$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.130$<br>$+0.03/^{\circ}\text{C}$ |

## Transmission Uncertainty (Specifications)

## Magnitude

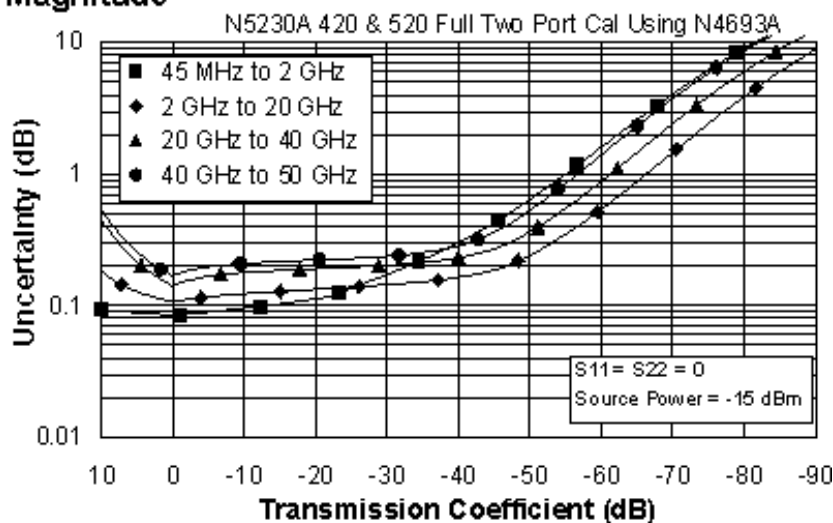


## Phase

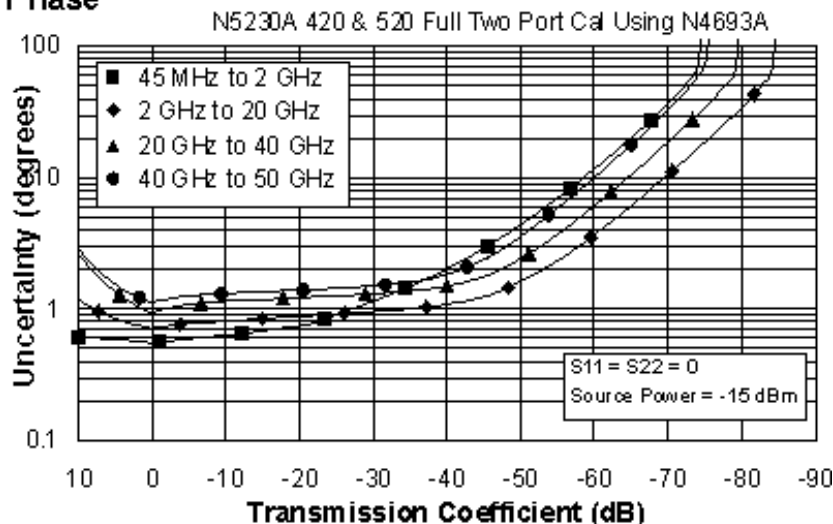


## Reflection Uncertainty (Specifications)

### Magnitude

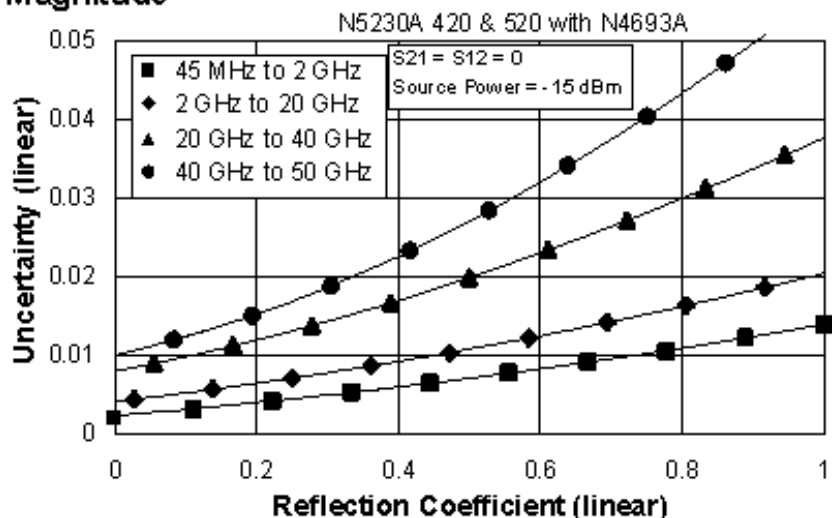

## Phase

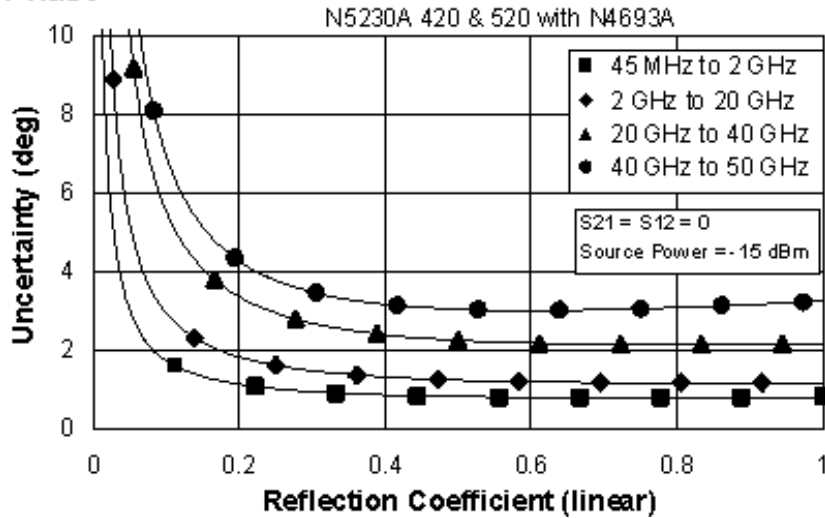

**Table 12.** N4693A Electronic Calibration Module  
N5230A - Option 425 or 525 (Configurable Test Set and Extended Power Range)


Applies to the N5230A Option 425 or 525 analyzers, N4693A(2.4mm) Electronic Calibration Module, 85133F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 45 MHz to<br>2 GHz                      | 2 to<br>20 GHz                          | 20 to<br>40 GHz                         | 40 to<br>50 GHz                         |
| Directivity           | 55                                      | 49                                      | 43                                      | 41                                      |
| Source Match          | 46                                      | 42                                      | 35                                      | 30                                      |
| Load Match            | 43                                      | 41                                      | 37                                      | 36                                      |
| Reflection Tracking   | $\pm 0.030$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.040$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.060$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.080$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.056$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.078$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.107$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.130$<br>$+0.03/^{\circ}\text{C}$ |

## Transmission Uncertainty (Specifications)

## Magnitude

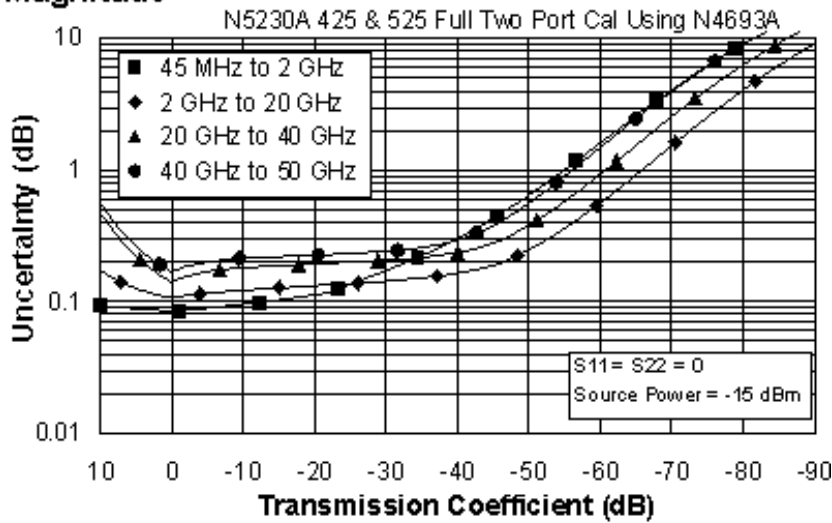


## Phase

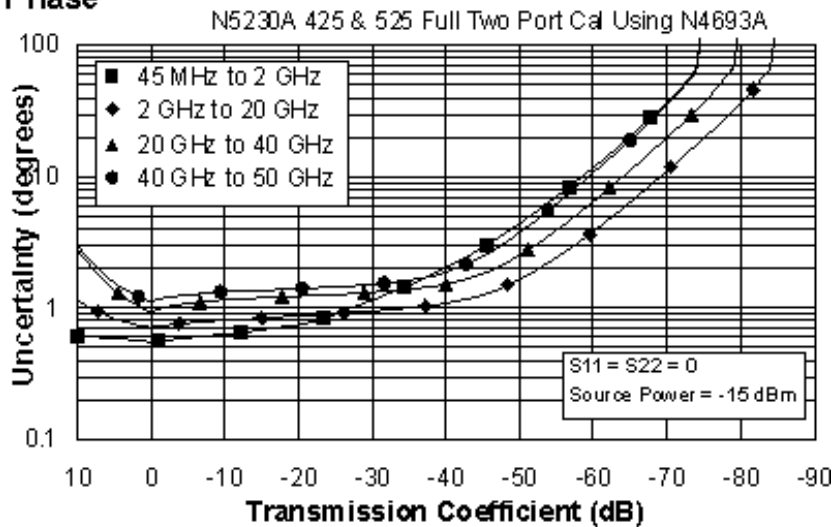


## Reflection Uncertainty (Specifications)

### Magnitude

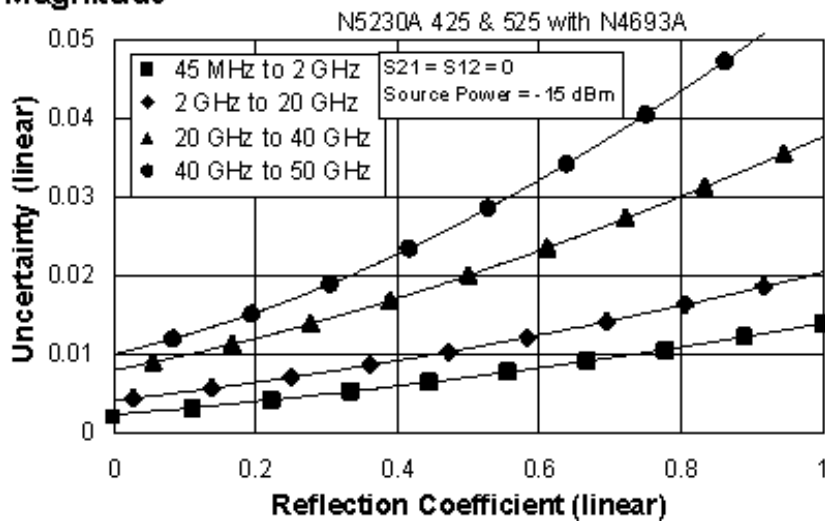

## Phase

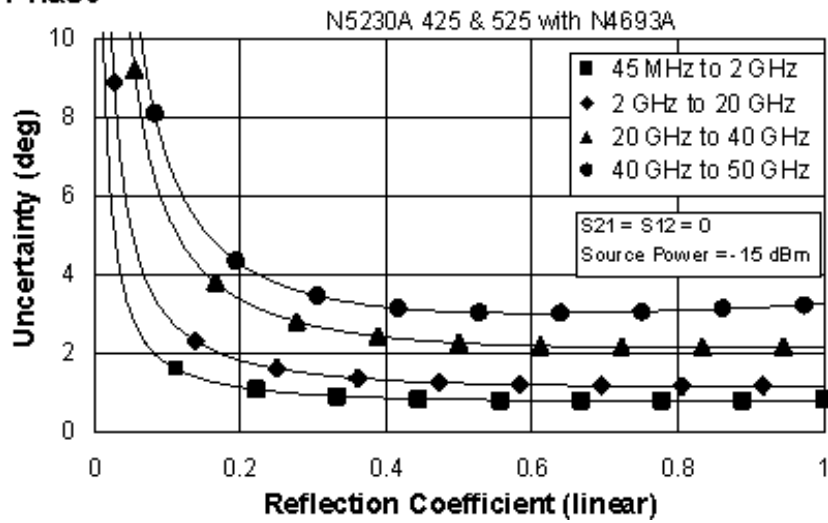

This N5230A document does not present specifications for the 85056D or 85056K Calibration Kit. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the data and curves for the 85056D and 85056K Calibration Kit or your PNA setup. View the [equations](#) used to generate the uncertainty curves.

## E8363/4B Corrected System Performance with WR-28 Connectors

### R11644A Calibration Kit:

#### Standard Configuration and Standard Power Range (E8363/4B)


#### Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

**Table 25.** R11644A Calibration Kit  
Standard Configuration and Standard Power Range  
(E8363/4B)

Applies to the, E8363/4B analyzers, R11644A (WR-28) calibration kit, 85133F flexible test port cable set with the R281A and R281B launch sets, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23 \pm 3 \text{ }^\circ\text{C}$ , with  $< 1 \text{ }^\circ\text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                    |
|-----------------------|---------------------------------------|
|                       | 26.5 to<br>40 GHz                     |
| Directivity           | 50                                    |
| Source Match          | 50                                    |
| Load Match            | 50                                    |
| Reflection Tracking   | $\pm 0.000$<br>$+0.03/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.018$<br>$+0.03/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications) Magnitude

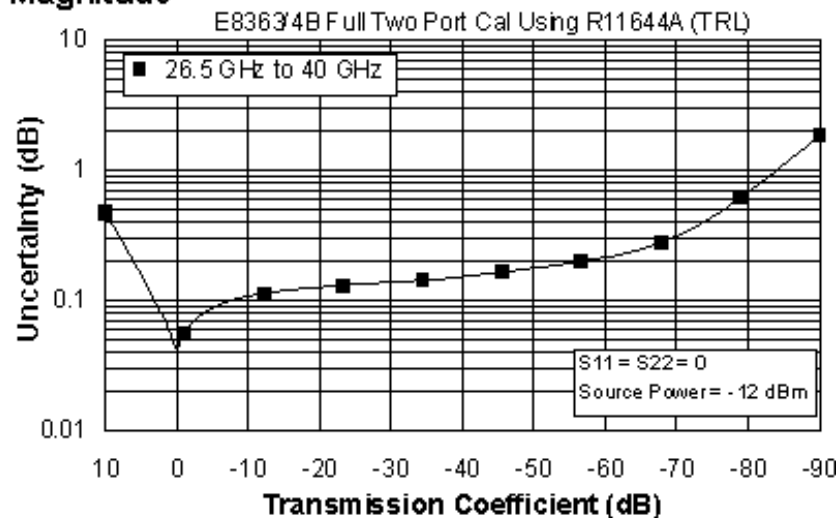




## Phase

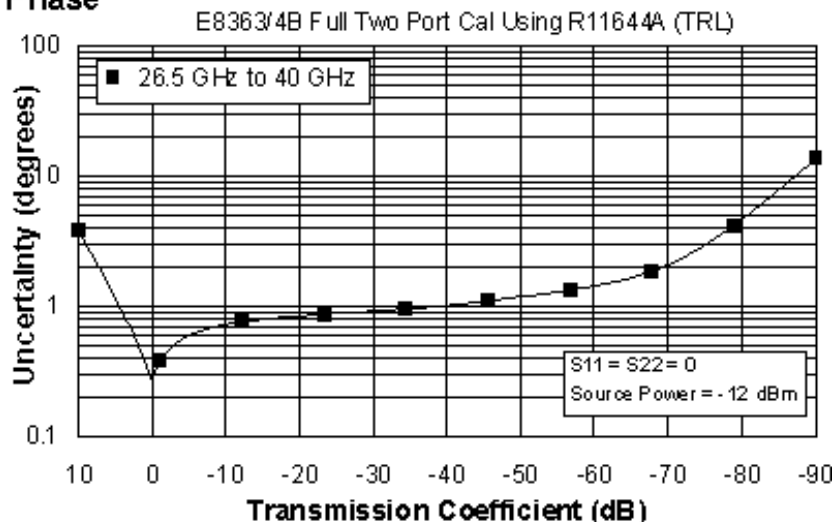


## Reflection Uncertainty (Specifications)

### Magnitude

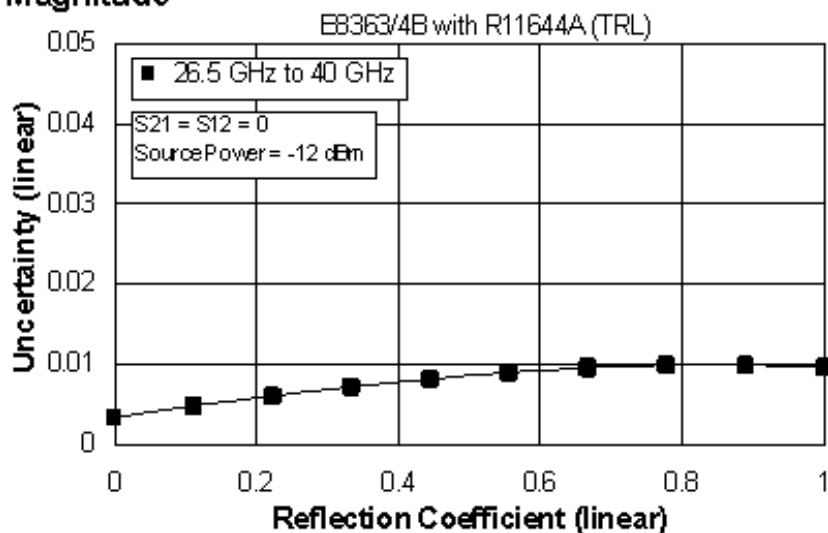

### Phase

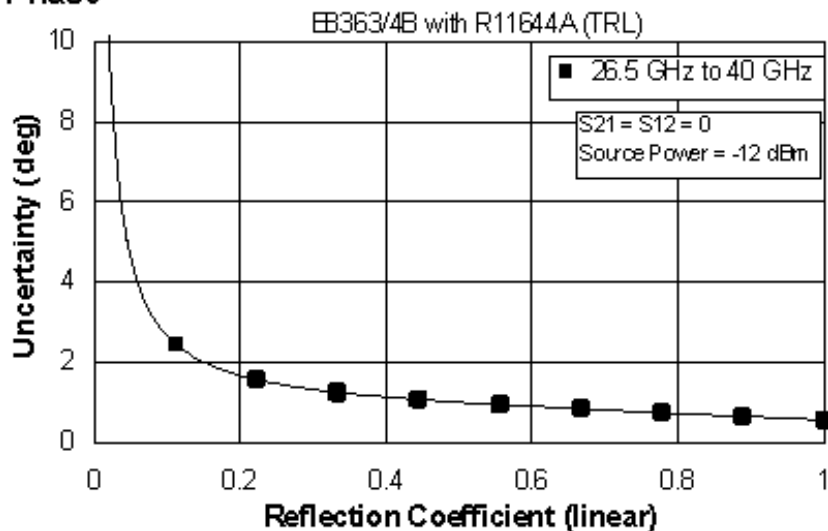

**Table 26.** R11644A Calibration Kit

Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E8363/4B analyzers, R11644A (WR-28) calibration kit, 85133F flexible test port cable set with the R281A and R281B launch sets, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB)    |
|-----------------------|-----------------------|
|                       | <b>26.5 to 40 GHz</b> |
| Directivity           | 50                    |
| Source Match          | 50                    |
| Load Match            | 50                    |
| Reflection Tracking   | ±0.000<br>+0.03/°C    |
| Transmission Tracking | ±0.019<br>+0.03/°C    |

**Transmission Uncertainty (Specifications)**

**Magnitude**

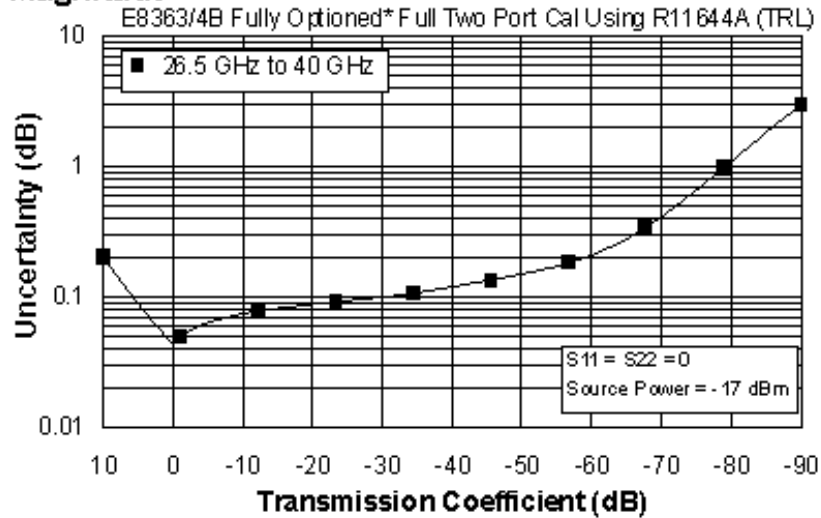


### Phase

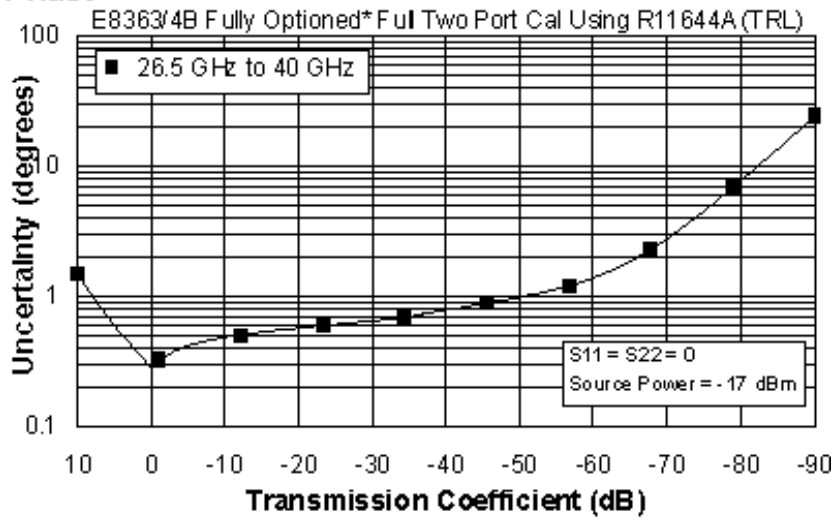


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

### Reflection Uncertainty (Specifications)

#### Magnitude

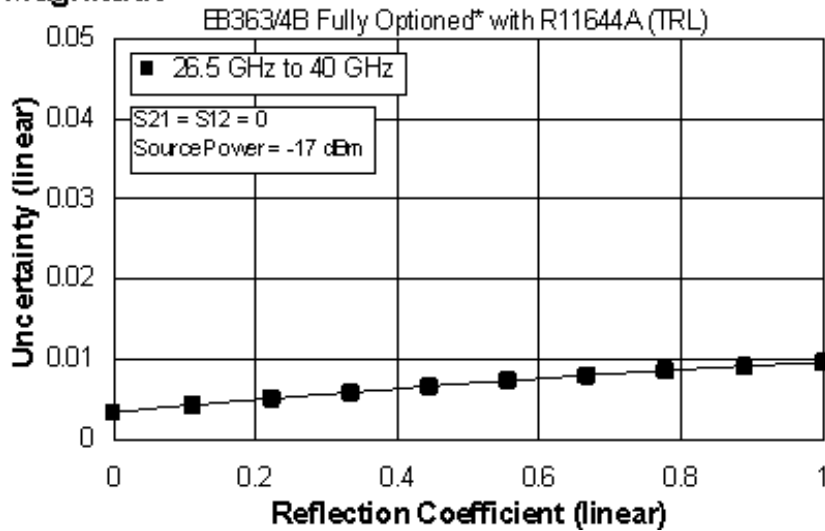

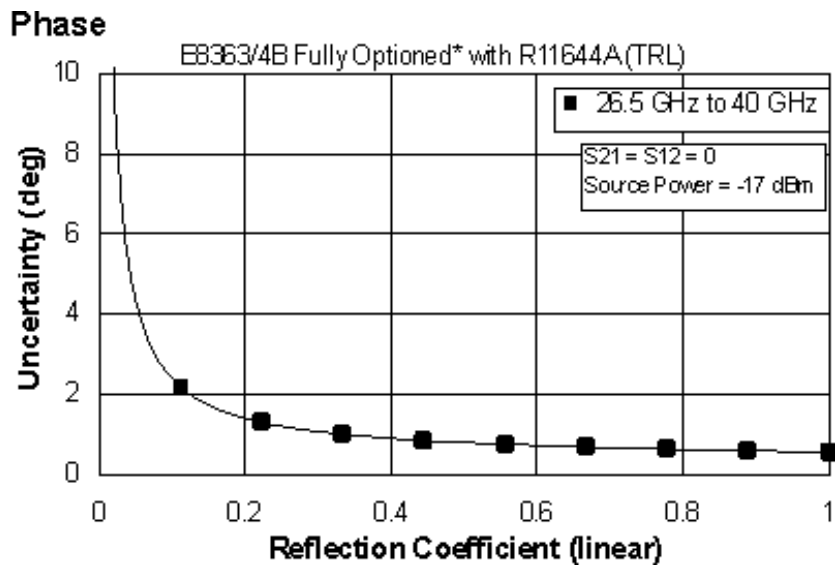

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## E8363/4B Corrected System Performance with 2.92mm Connectors

### 85056K Calibration Kit:

#### Standard Configuration and Standard Power Range (E8363/4B)


#### Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

**Table 7.** 85056K Calibration Kit  
Standard Configuration and Standard Power Range  
(E8363/4B)


Applies to the, E8363/4B analyzers, 85056K (2.92mm) calibration kit, 85133F flexible test port cable set, and a full 2-port calibration.  
Also applies to the following condition:  
Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 0.045 to<br>2 GHz                       | 2 to<br>20 GHz                          | 20 to<br>40 GHz                         |
| Directivity           | 42                                      | 42                                      | 40                                      |
| Source Match          | 40                                      | 40                                      | 35                                      |
| Load Match            | 42                                      | 41                                      | 38                                      |
| Reflection Tracking   | $\pm 0.018$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.018$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.067$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.011$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.042$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.089$<br>$+0.03/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications) Magnitude

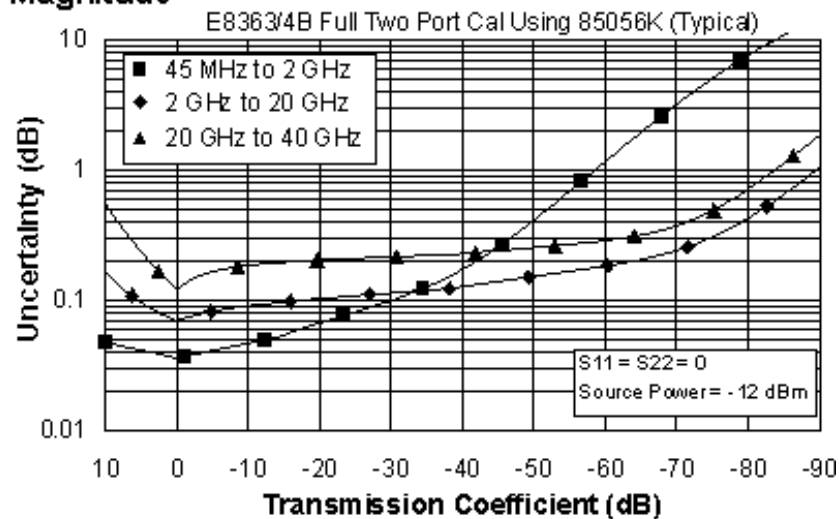


### Phase

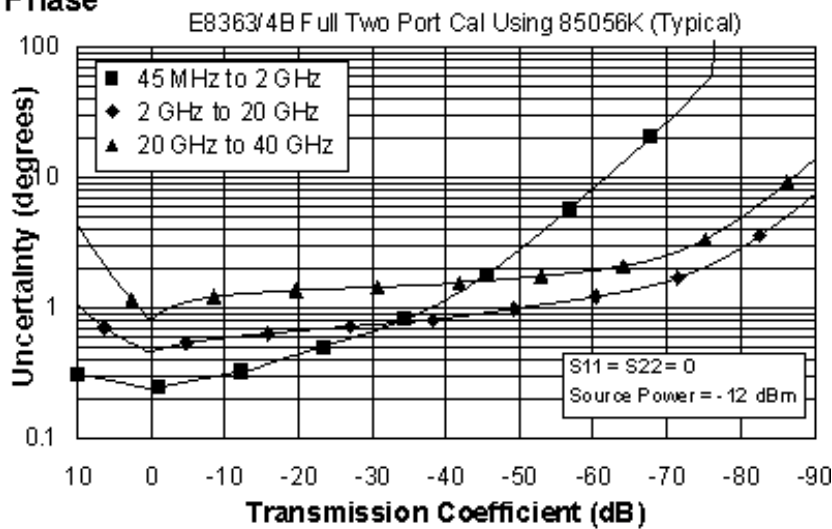

### Reflection Uncertainty (Specifications)

#### Magnitude

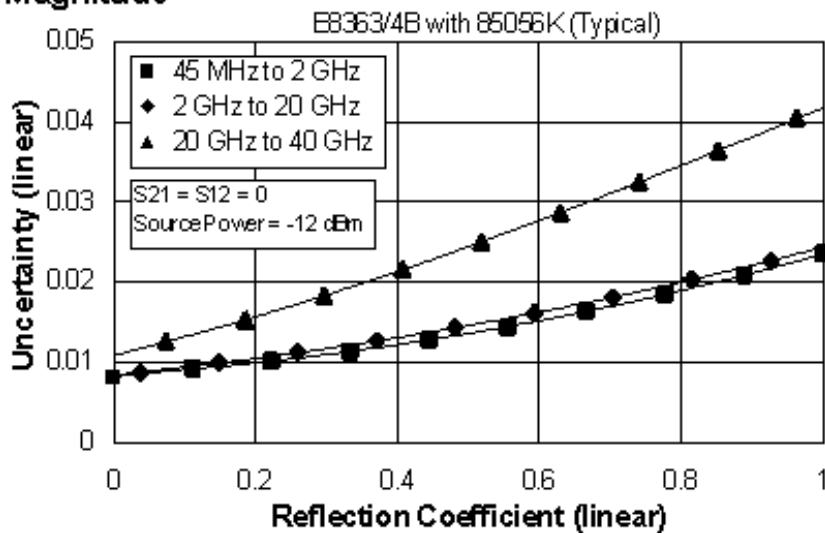

#### Phase

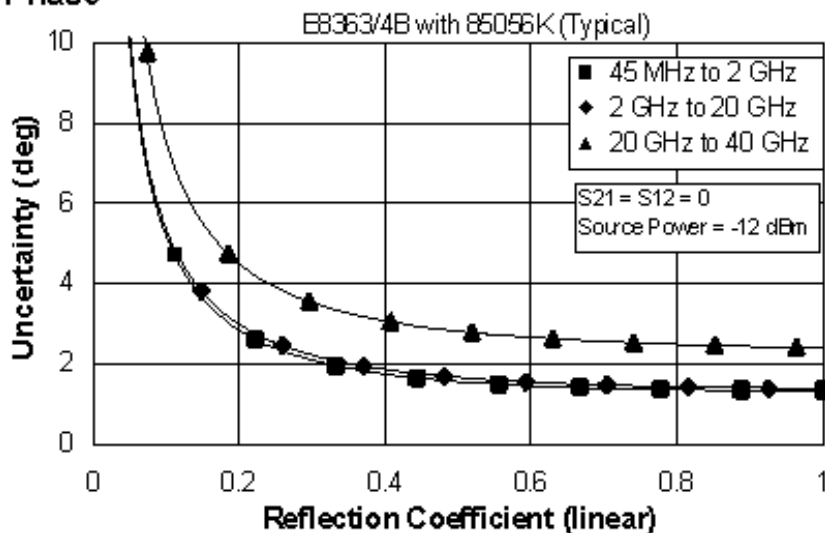


Table 8. 85056K Calibration Kit

## Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E8363/4B analyzers, 85056K (2.92mm) calibration kit, 85133F flexible test port cable set, and a full 2-port calibration.

Also applies to the following condition:


Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 0.045 to<br>2 GHz                       | 2 to<br>20 GHz                          | 20 to<br>40 GHz                         |
| Directivity           | 42                                      | 42                                      | 40                                      |
| Source Match          | 40                                      | 40                                      | 35                                      |
| Load Match            | 42                                      | 41                                      | 38                                      |
| Reflection Tracking   | $\pm 0.018$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.018$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.067$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.021$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.046$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.094$<br>$+0.03/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications Magnitude)

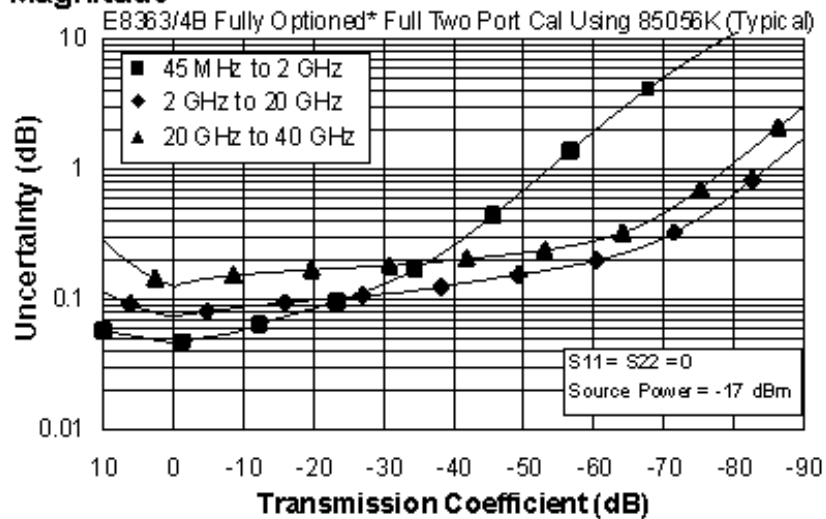


## Phase

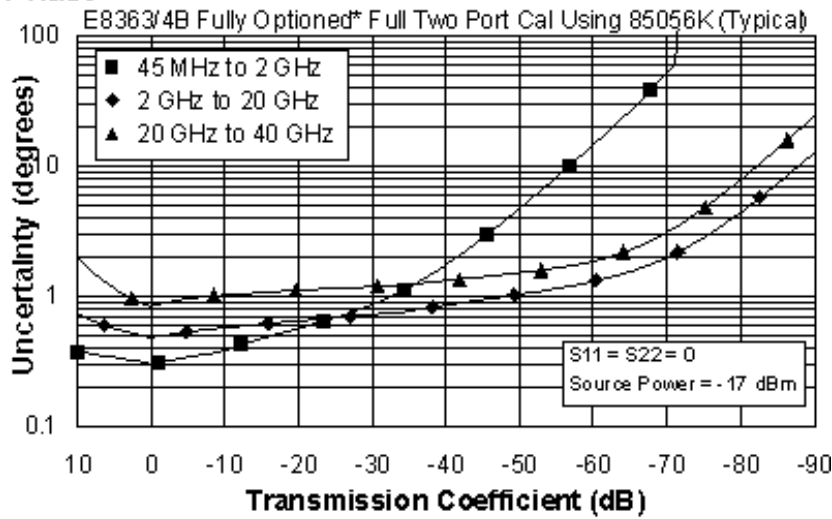


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

### Magnitude

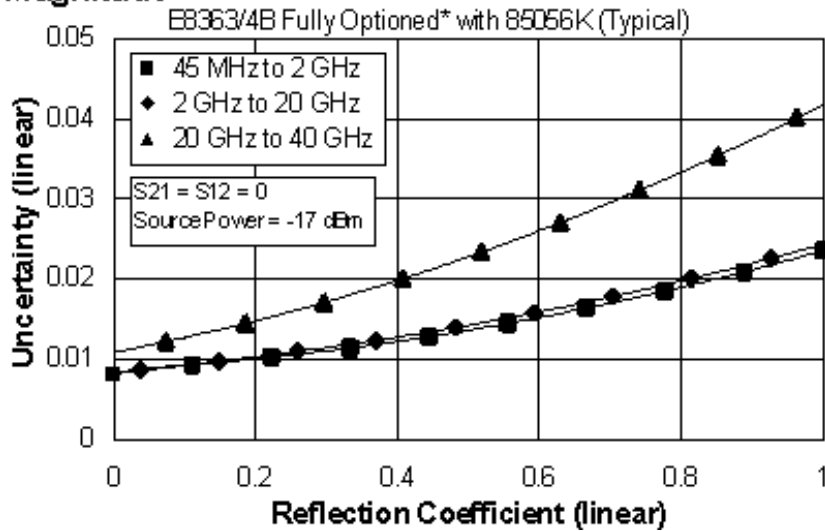



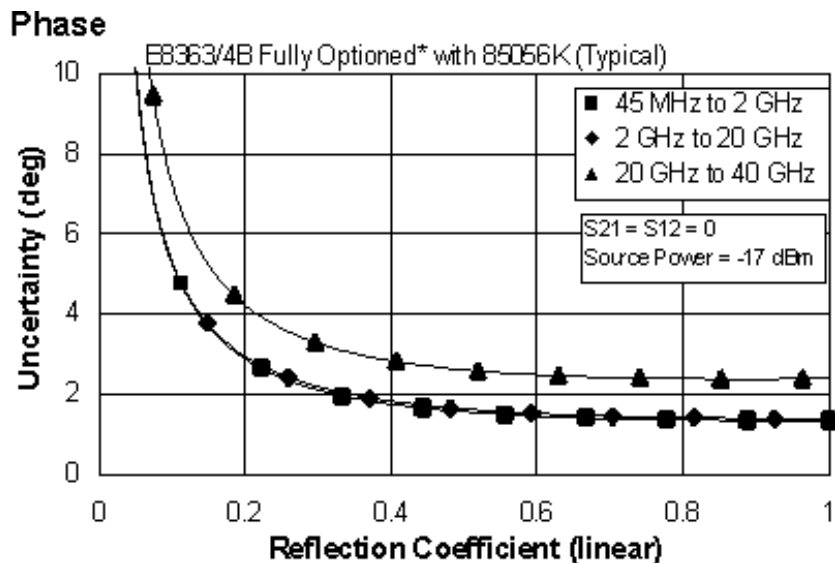

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## E836xB Corrected System Performance with 3.5mm Connectors

---

### 85052B Calibration Kit:

Standard Configuration and Standard Power Range (E836xB)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
(E836xB - Option 014, UNL, 016, 080, and 081)

### 85052C Calibration Kit:

Standard Configuration and Standard Power Range (E836xB)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
(E836xB - Option 014, UNL, 016, 080, and 081)

### 85052D Calibration Kit:

Standard Configuration and Standard Power Range (E836xB)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
(E836xB - Option 014, UNL, 016, 080, and 081)

---


### **Table 9.** 85052B Calibration Kit Standard Configuration and Standard Power Range (E836xB)

Applies to the, E836xB analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:


↑ applies to the following condition:  
 Environmental temperature  $23 \pm 3 \text{ }^\circ\text{C}$ , with  $< 1 \text{ }^\circ\text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                    |                                       |                                       |
|-----------------------|---------------------------------------|---------------------------------------|---------------------------------------|
|                       | 45 MHz to 2 GHz                       | 2 to 20 GHz                           | 20 to 26.5 GHz                        |
| Directivity           | 48                                    | 44                                    | 44                                    |
| Source Match          | 40                                    | 31                                    | 31                                    |
| Load Match            | 48                                    | 44                                    | 44                                    |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^\circ\text{C}$ | $\pm 0.006$<br>$+0.02/^\circ\text{C}$ | $\pm 0.006$<br>$+0.03/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.009$<br>$+0.02/^\circ\text{C}$ | $\pm 0.088$<br>$+0.02/^\circ\text{C}$ | $\pm 0.104$<br>$+0.03/^\circ\text{C}$ |


### Transmission Uncertainty (Specifications) Magnitude

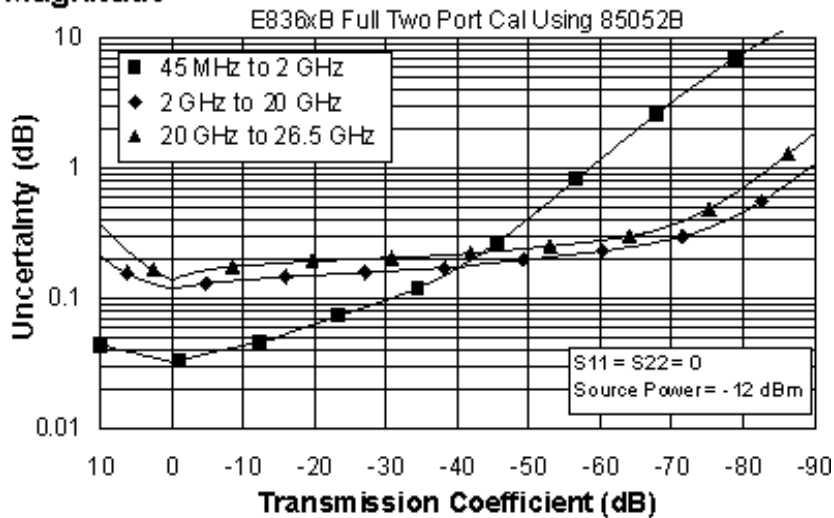


### Phase

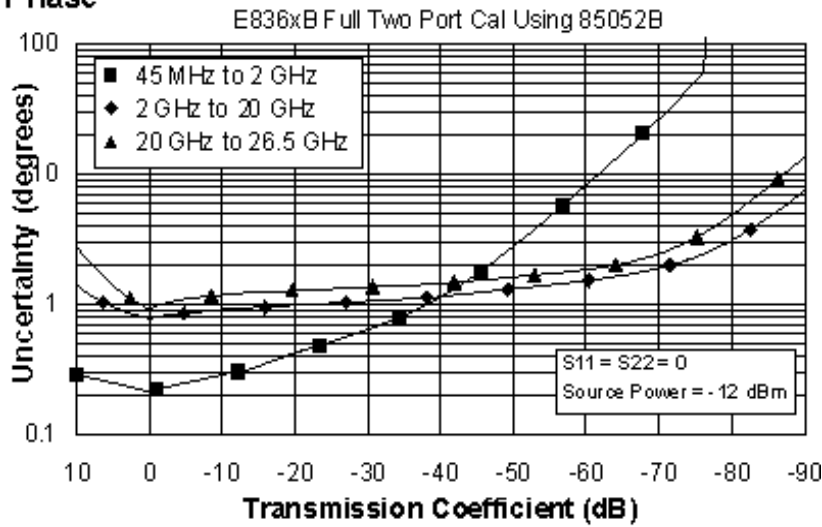

### Reflection Uncertainty (Specifications) Magnitude

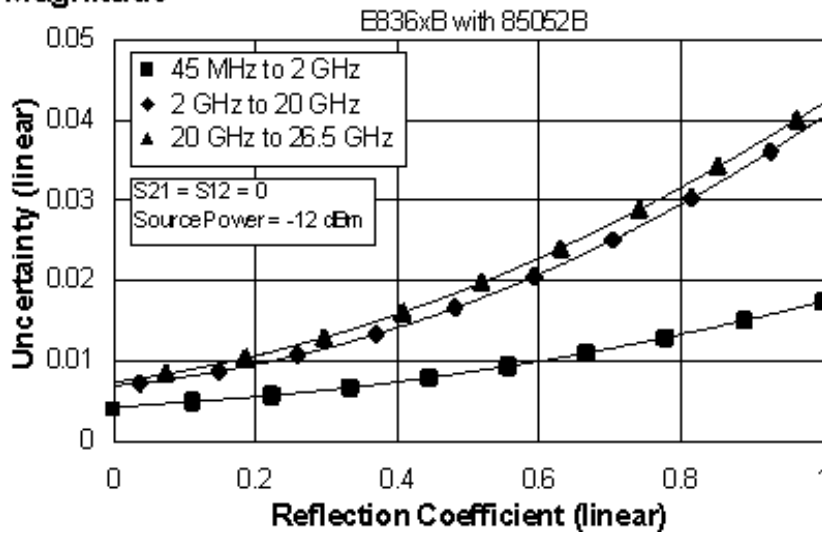

### Phase

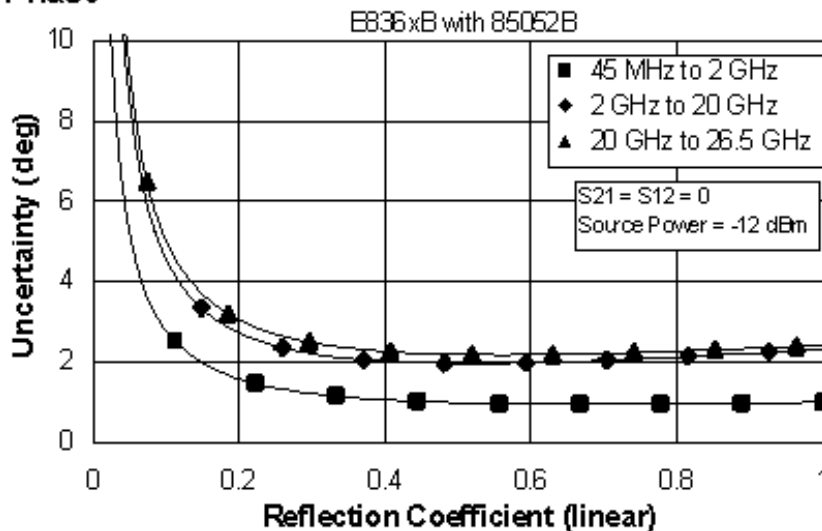


**Table 10.** 85052B Calibration Kit  
Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E836xB analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 45 MHz to 2 GHz                         | 2 to 20 GHz                             | 20 to 26.5 GHz                          |
| Directivity           | 48                                      | 44                                      | 44                                      |
| Source Match          | 40                                      | 31                                      | 31                                      |
| Load Match            | 48                                      | 44                                      | 44                                      |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.006$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.006$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.017$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.091$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.106$<br>$+0.03/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications) Magnitude

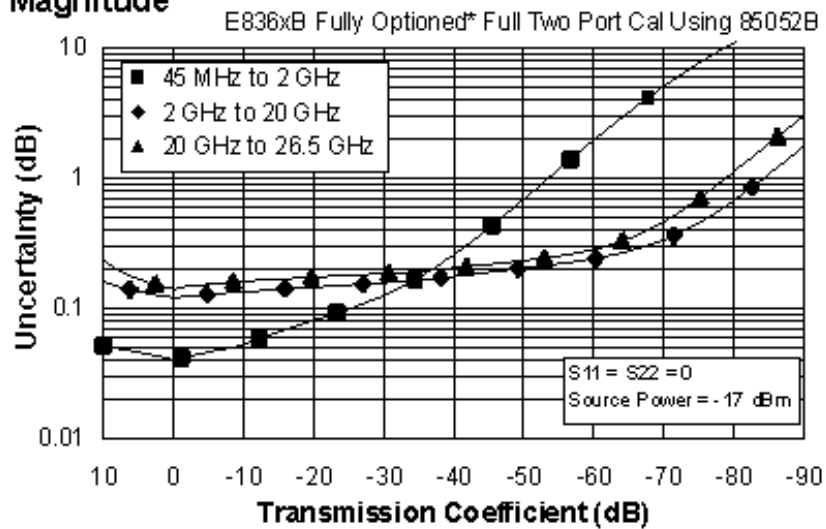


## Phase

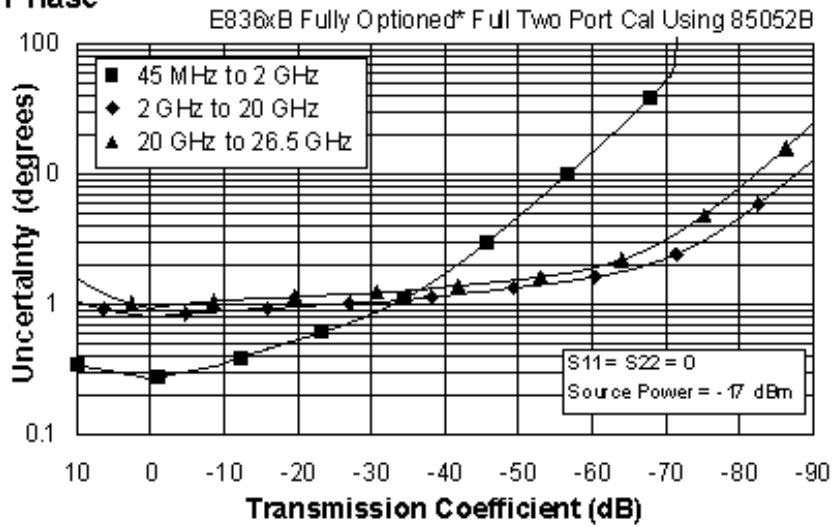


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
(E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

### Magnitude

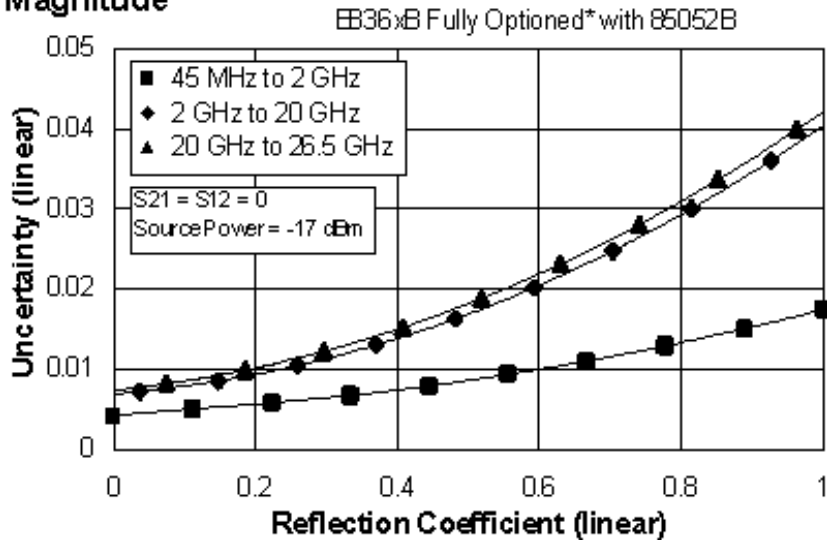

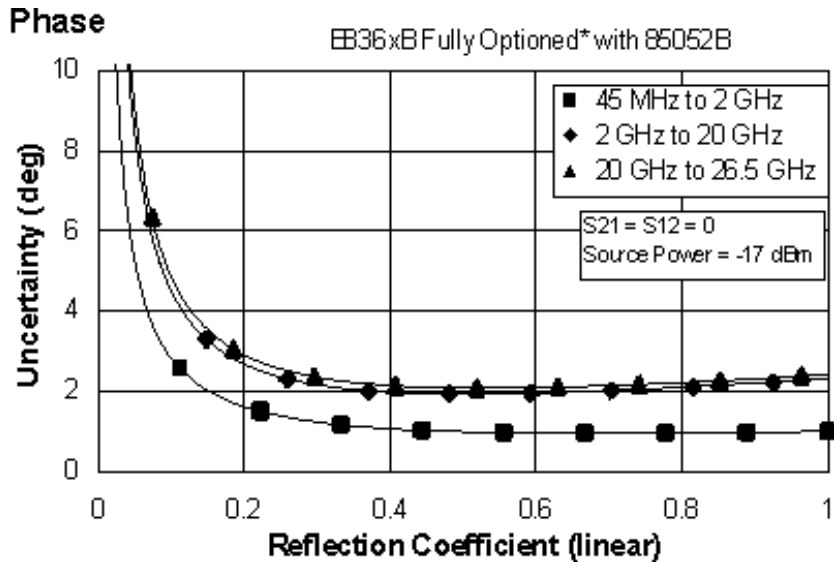

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
(E836xB - Option 014, UNL, 016, 080, and 081)


**Table 11. 85052C Calibration Kit**  
Standard Configuration and Standard Power Range  
(E836xB)

Applies to the, E836xB analyzers, 85052C (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to 2 GHz    | 2 to 20 GHz        | 20 to 26.5 GHz     |
| Directivity           | 48                 | 50                 | 50                 |
| Source Match          | 40                 | 50                 | 50                 |
| Load Match            | 48                 | 50                 | 50                 |
| Reflection Tracking   | ±0.003<br>+0.02/°C | ±0.000<br>+0.02/°C | ±0.000<br>+0.03/°C |
| Transmission Tracking | ±0.009<br>+0.02/°C | ±0.014<br>+0.02/°C | ±0.018<br>+0.03/°C |

### Transmission Uncertainty (Specifications)

## Magnitude

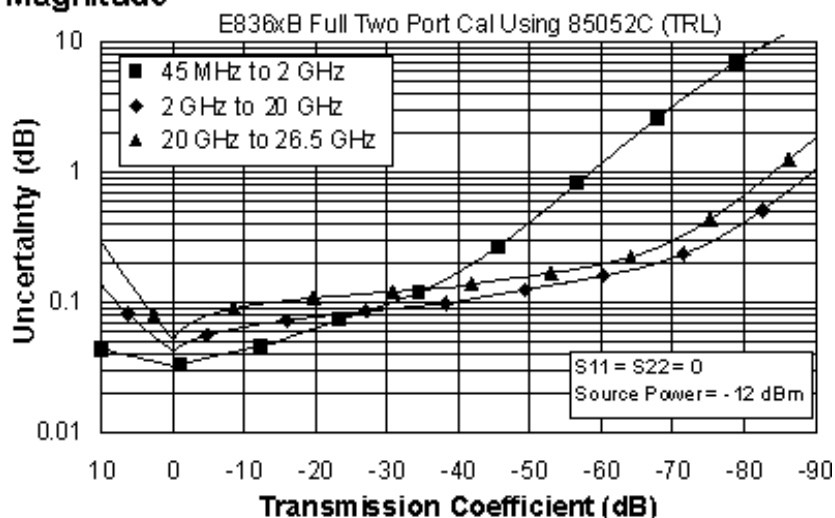


## Phase

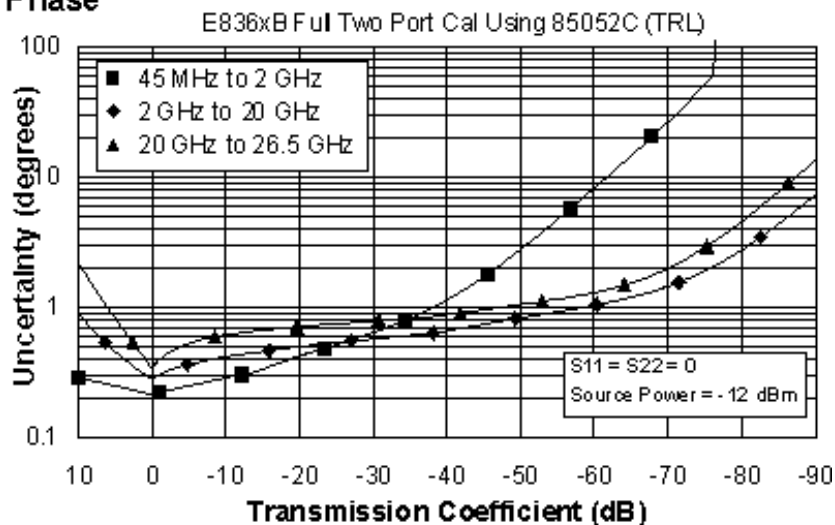


## Reflection Uncertainty (Specifications)

### Magnitude

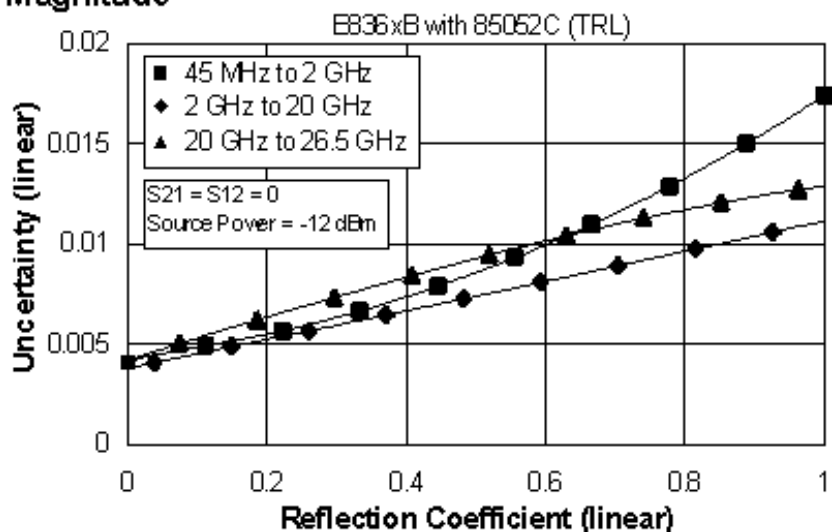



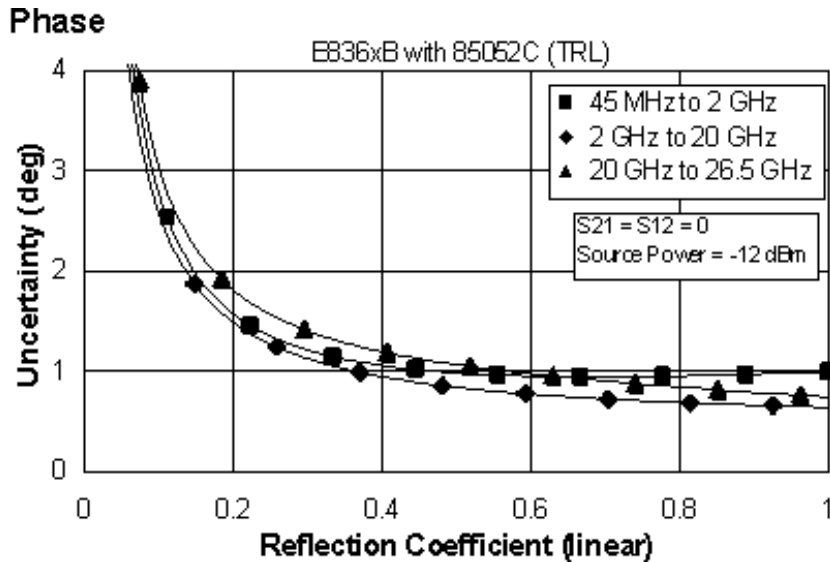

**Table 12. 85052C Calibration Kit**

Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)


Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E836xB analyzers, 85052C (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to 2 GHz    | 2 to 20 GHz        | 20 to 26.5 GHz     |
| Directivity           | 48                 | 50                 | 50                 |
| Source Match          | 40                 | 50                 | 50                 |
| Load Match            | 48                 | 50                 | 50                 |
| Reflection Tracking   | ±0.003<br>+0.02/°C | ±0.000<br>+0.02/°C | ±0.000<br>+0.03/°C |
| Transmission Tracking | ±0.017<br>+0.02/°C | ±0.016<br>+0.02/°C | ±0.019<br>+0.03/°C |

**Transmission Uncertainty (Specifications)**

## Magnitude

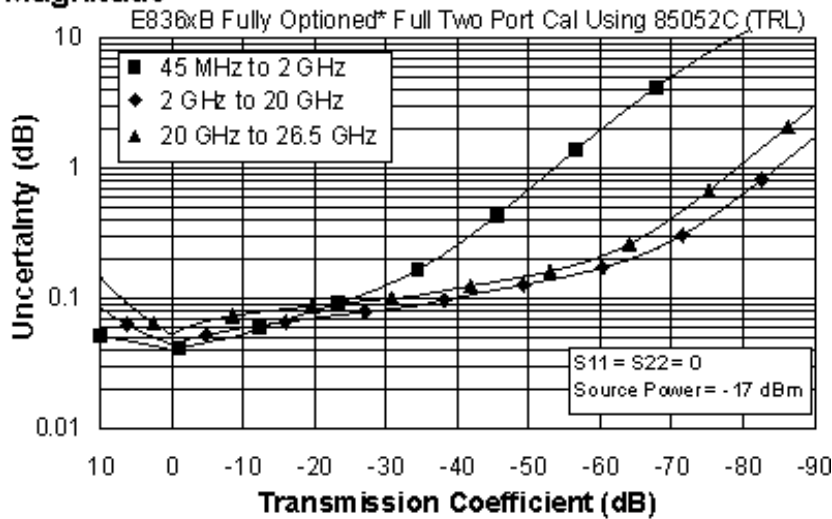


## Phase

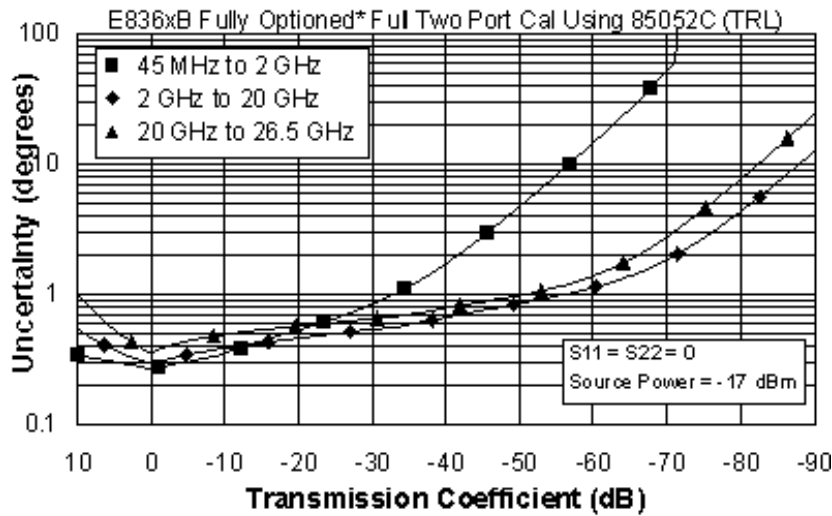


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

## Magnitude

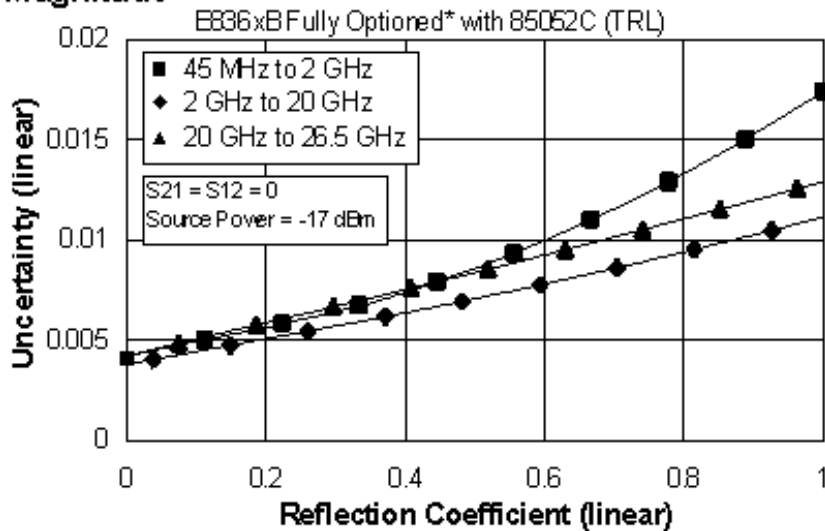

## Phase

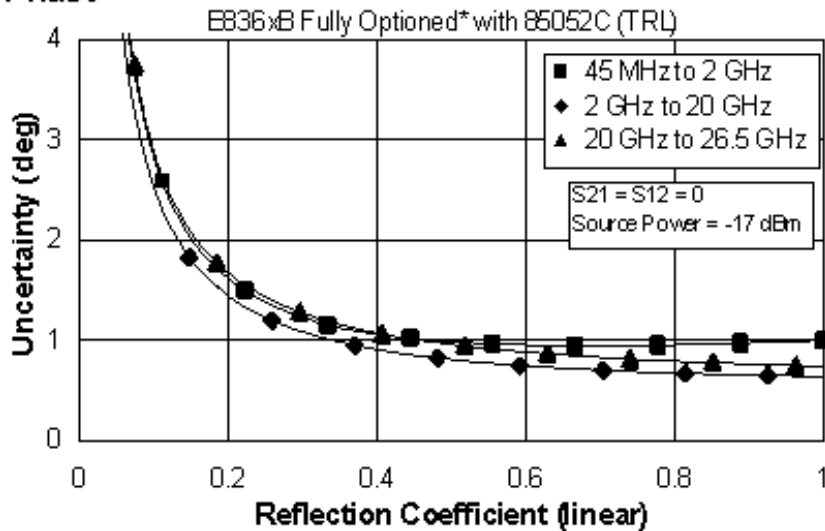

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)


### Table 13. 85052D Calibration Kit

Standard Configuration and Standard Power Range (E836xB)


Applies to the, E836xB analyzers, 85052D (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB)                    |                                       |                                       |
|-----------------------|---------------------------------------|---------------------------------------|---------------------------------------|
|                       | 45 MHz to 2 GHz                       | 2 to 20 GHz                           | 20 to 26.5 GHz                        |
| Directivity           | 42                                    | 36                                    | 30                                    |
| Source Match          | 37                                    | 28                                    | 25                                    |
| Load Match            | 42                                    | 36                                    | 30                                    |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^\circ\text{C}$ | $\pm 0.008$<br>$+0.02/^\circ\text{C}$ | $\pm 0.011$<br>$+0.03/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.014$<br>$+0.02/^\circ\text{C}$ | $\pm 0.131$<br>$+0.02/^\circ\text{C}$ | $\pm 0.250$<br>$+0.03/^\circ\text{C}$ |


### Transmission Uncertainty (Specifications) Magnitude

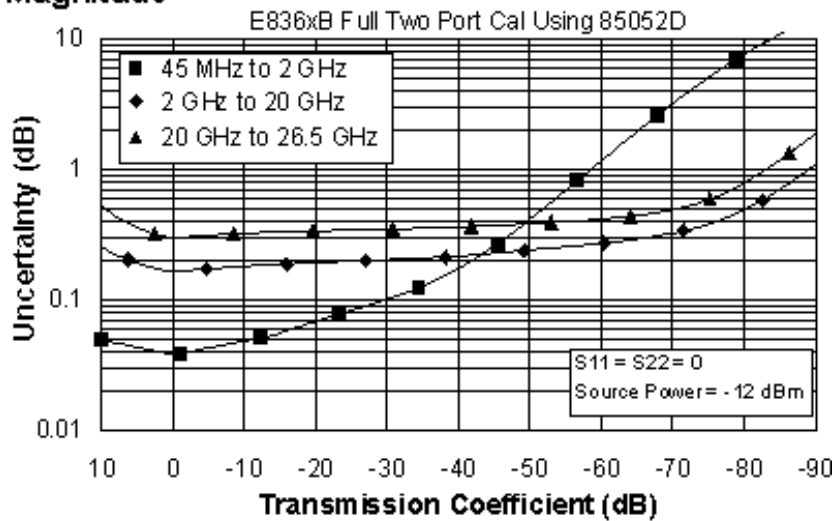


### Phase

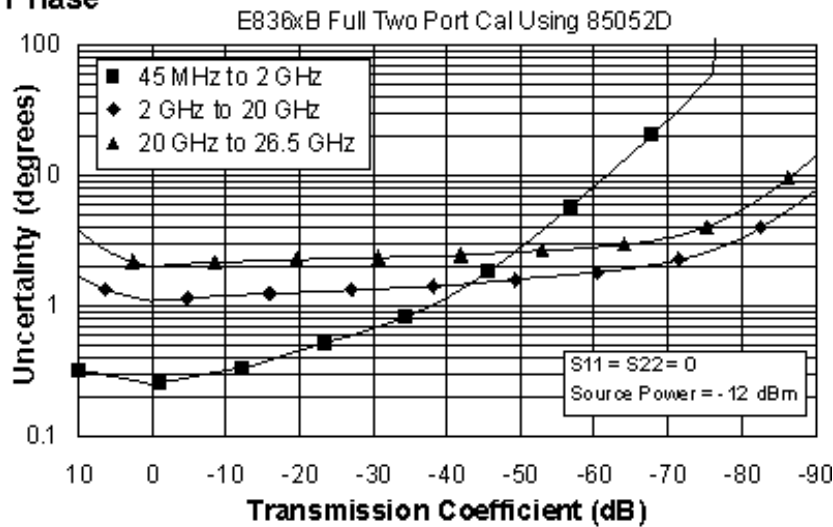

**Reflection Uncertainty (Specifications)**  
**Magnitude**

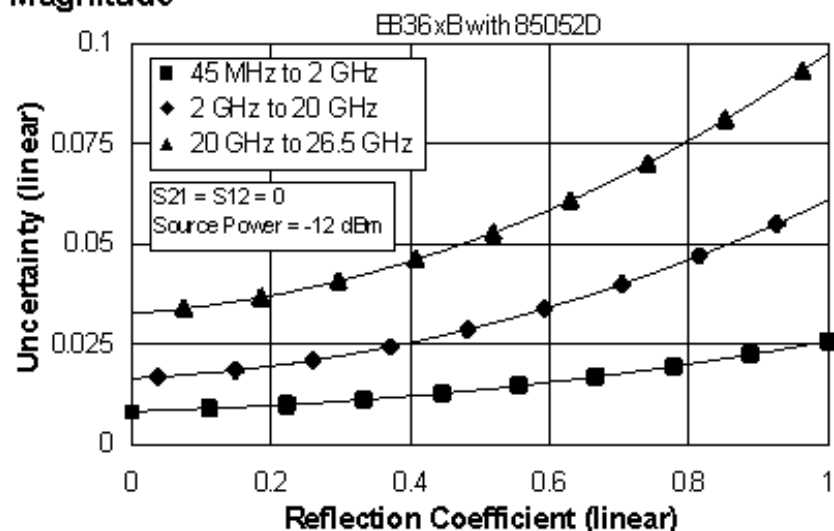

**Phase**

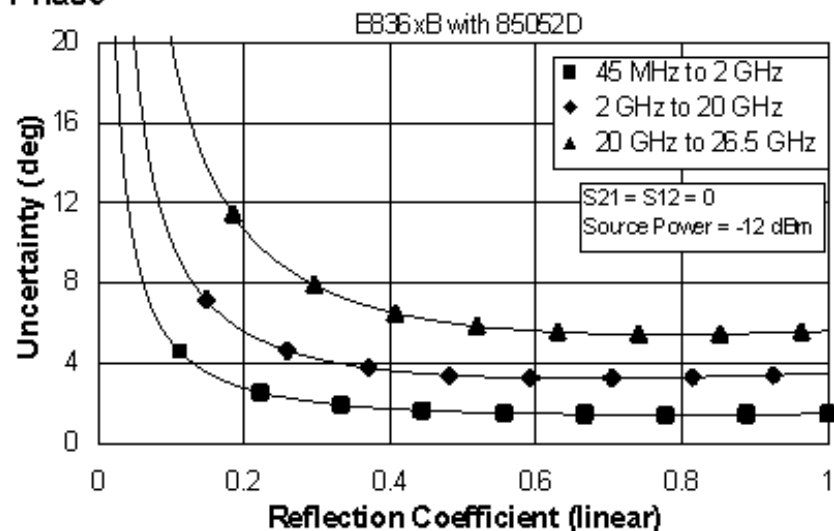

**Table 14. 85052D Calibration Kit**

Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)


Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E836xB analyzers, 85052D (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                    |                                       |                                       |
|-----------------------|---------------------------------------|---------------------------------------|---------------------------------------|
|                       | 45 MHz to 2 GHz                       | 2 to 20 GHz                           | 20 to 26.5 GHz                        |
| Directivity           | 42                                    | 36                                    | 30                                    |
| Source Match          | 37                                    | 28                                    | 25                                    |
| Load Match            | 42                                    | 36                                    | 30                                    |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^\circ\text{C}$ | $\pm 0.008$<br>$+0.02/^\circ\text{C}$ | $\pm 0.011$<br>$+0.03/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.026$<br>$+0.02/^\circ\text{C}$ | $\pm 0.138$<br>$+0.02/^\circ\text{C}$ | $\pm 0.261$<br>$+0.03/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

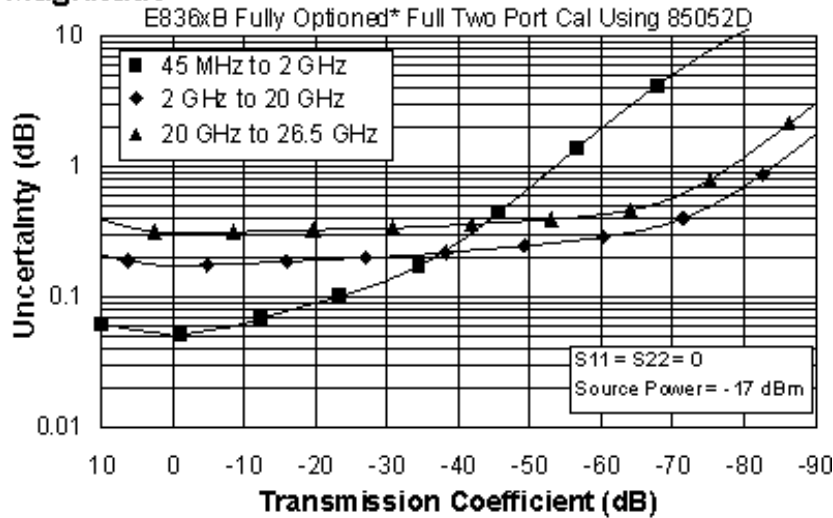


#### Phase

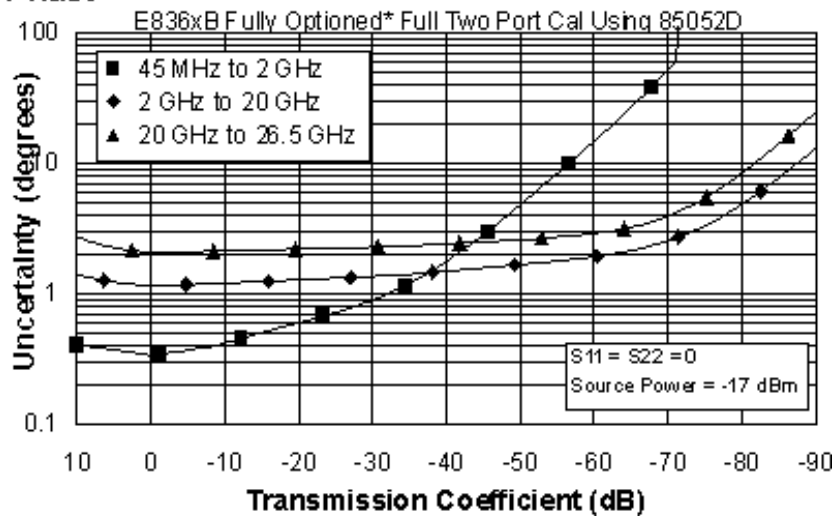


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
 (E836xB - Option 014, UNL, 016, 080, and 081)

**Reflection Uncertainty (Specifications)**  
**Magnitude**

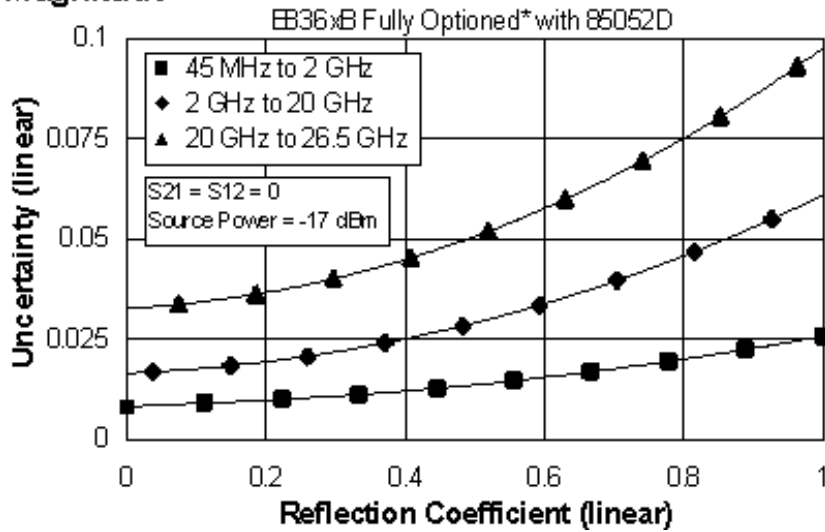

**Phase**

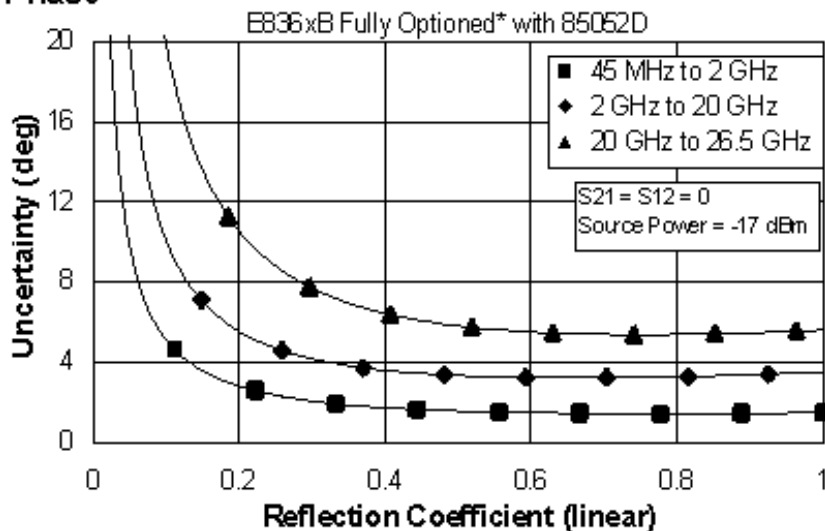

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
 (E836xB - Option 014, UNL, 016, 080, and 081)

## N5230A Corrected System Performance with 3.5mm Connectors

### Options 020/025, 120/125, 220/225, 420/425, and 520/525

Options 220/225, 420/425, 520/525: From 10 MHz to 45 MHz, performance is characterized as "typical". To generate these typical values, please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator).

### 85052B Calibration Kit

#### N5230A - Option 020/120

#### Standard Test Set and Standard Power Range

#### N5230A - Option 025/125

#### Configurable Test Set and Extended Power Range

#### N5230A - Option 220

#### Standard Test Set and Standard Power Range

#### N5230A Option 225

#### Configurable Test Set and Extended Power Range

### N4691A Electronic Calibration (ECal) Module

#### N5230A - Option 220

#### Standard Test Set and Standard Power Range

#### N5230A Option 225

#### Configurable Test Set and Extended Power Range

**Table 3.** 85052B Calibration Kit

### N5230A - Option 020/120 (Standard Test Set and Standard Power Range)

Applies to the N5230A Option 020/120 analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:


Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB)   |                    |                    |                    |
|-----------------------|----------------------|--------------------|--------------------|--------------------|
|                       | 300 kHz to<br>10 MHz | 10 MHz to<br>2 GHz | 2 GHz to<br>8 GHz  | 8 to<br>13.5 GHz   |
| Directivity           | 48                   | 48                 | 44                 | 44                 |
| Source Match          | 40                   | 40                 | 33                 | 31                 |
| Load Match            | 48                   | 48                 | 44                 | 44                 |
| Reflection Tracking   | ±0.003<br>+0.02/°C   | ±0.003<br>+0.02/°C | ±0.003<br>+0.03/°C | ±0.006<br>+0.03/°C |
| Transmission Tracking | ±0.017<br>+0.02/°C   | ±0.015<br>+0.02/°C | ±0.075<br>+0.03/°C | ±0.131<br>+0.03/°C |




## Transmission Uncertainty (Specifications)

### Magnitude

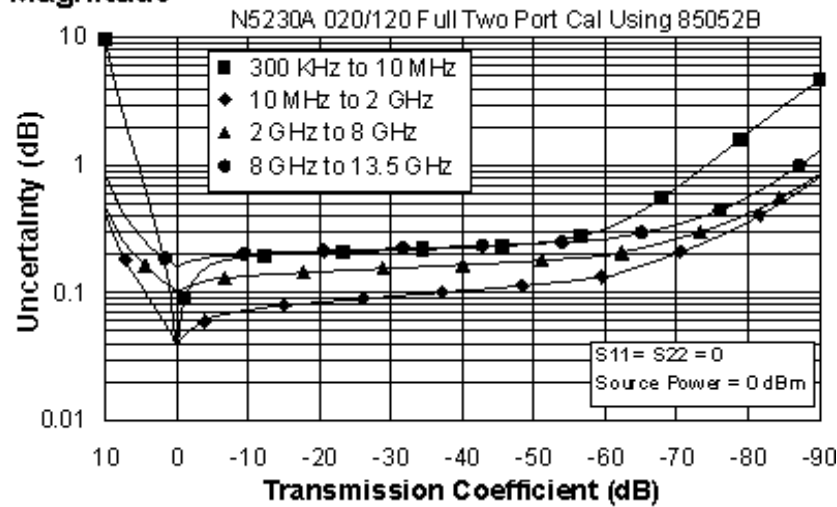


### Phase

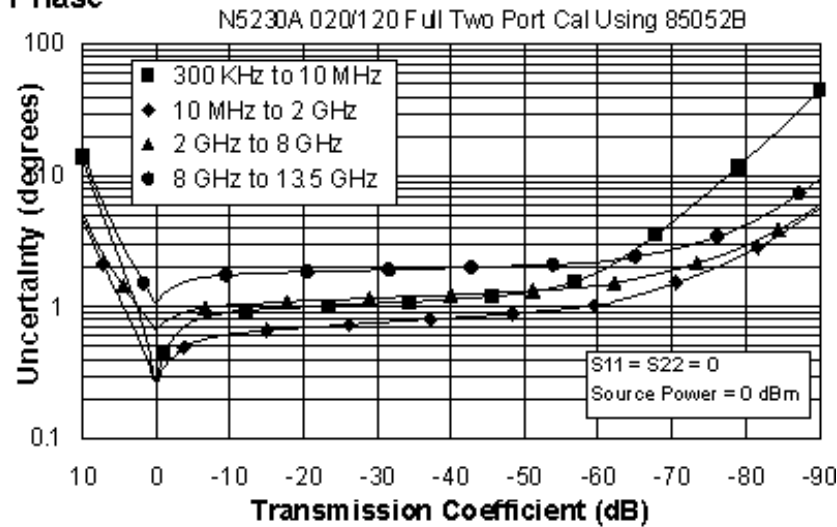


## Reflection Uncertainty (Specifications)

## Magnitude

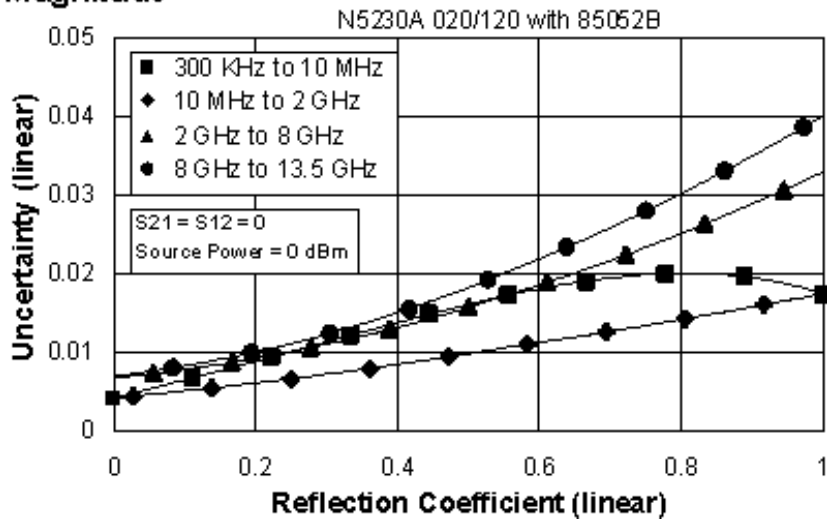

## Phase

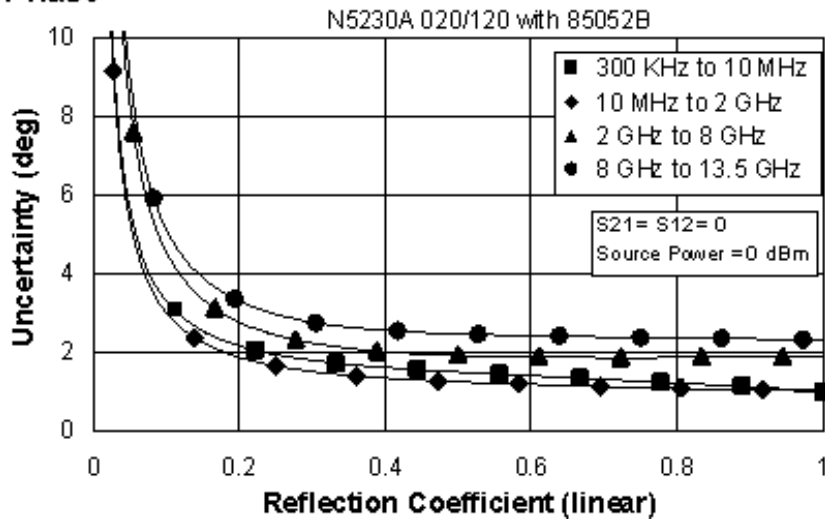

**Table 4.** 85052B Calibration Kit

### N5230A - Option 025/125 (Configurable Test Set and Extended Power Range)


Applies to the N5230A Option 025/125 analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 300 kHz to 10 MHz                       | 10 MHz to 2 GHz                         | 2 GHz to 8 GHz                          | 8 to 13.5 GHz                           |
| Directivity           | 48                                      | 48                                      | 44                                      | 44                                      |
| Source Match          | 40                                      | 40                                      | 33                                      | 31                                      |
| Load Match            | 48                                      | 48                                      | 44                                      | 44                                      |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.003$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.003$<br>$+0.03/^{\circ}\text{C}$ | $\pm 0.006$<br>$+0.03/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.017$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.015$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.075$<br>$+0.03/^{\circ}\text{C}$ | $\pm 0.131$<br>$+0.03/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

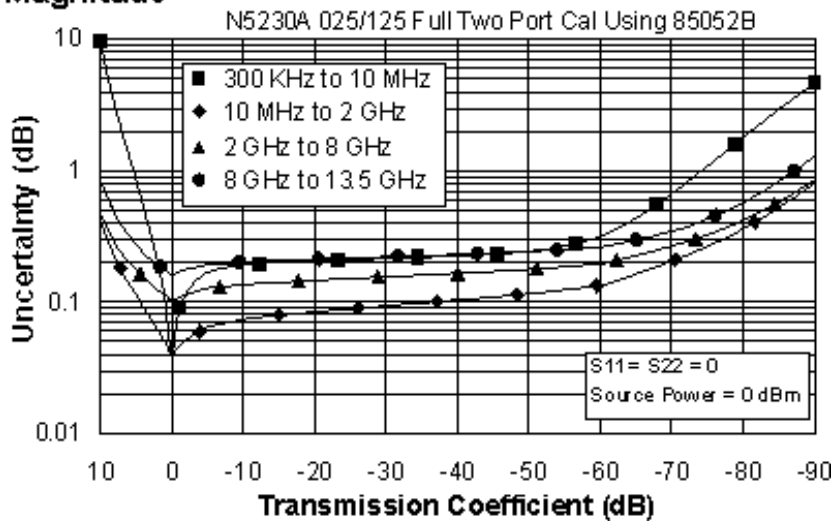


### Phase

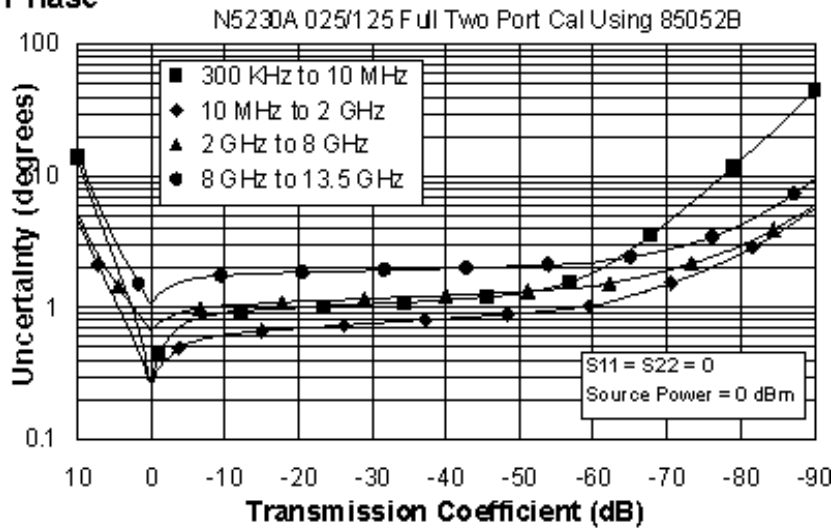


### Reflection Uncertainty (Specifications)

#### Magnitude

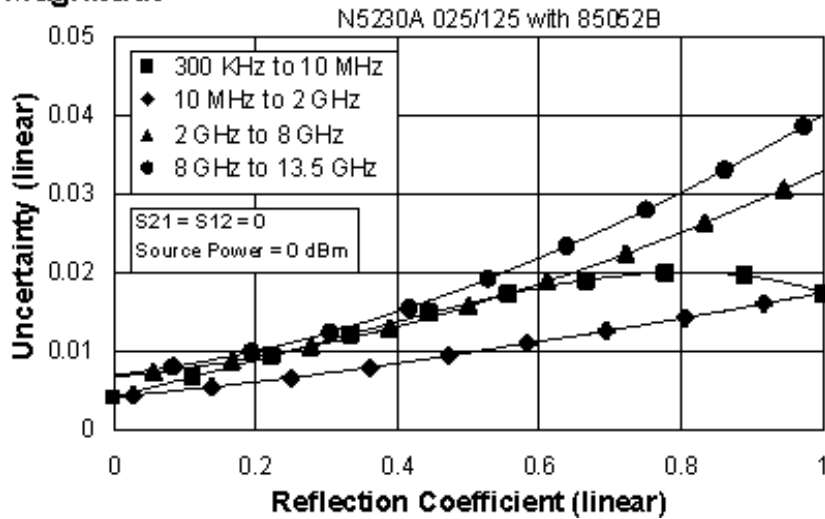

#### Phase

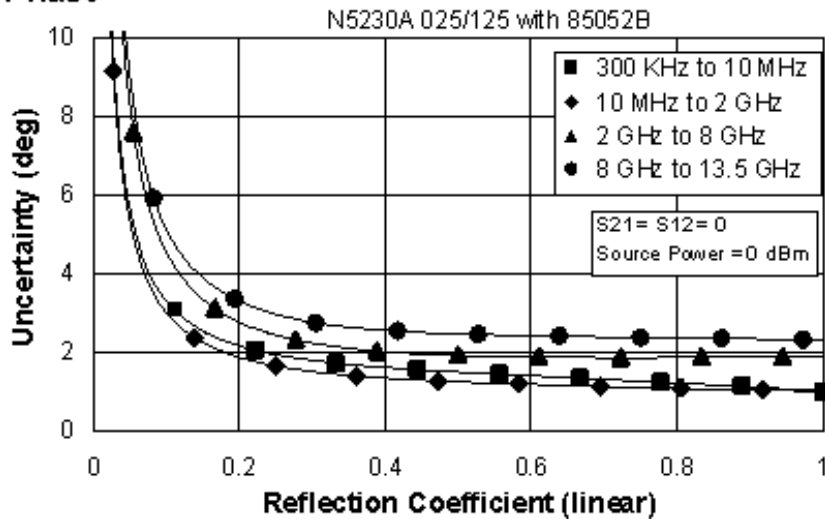

**Table 5. 85052B Calibration Kit**  
**N5230A - Option 220 (Standard Test Set and Standard Power Range)**


Applies to the, N5230A Option 220 analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to 500 MHz  | 500 MHz to 2 GHz   | 2 to 8 GHz         | 8 to 20 GHz        |
| Directivity           | 48                 | 48                 | 44                 | 44                 |
| Source Match          | 40                 | 40                 | 33                 | 31                 |
| Load Match            | 48                 | 48                 | 44                 | 44                 |
| Reflection Tracking   | ±0.003<br>+0.02/°C | ±0.003<br>+0.02/°C | ±0.003<br>+0.03/°C | ±0.006<br>+0.03/°C |
| Transmission Tracking | ±0.010<br>+0.02/°C | ±0.014<br>+0.02/°C | ±0.062<br>+0.03/°C | ±0.104<br>+0.03/°C |

**Transmission Uncertainty (Specifications)**

**Magnitude**

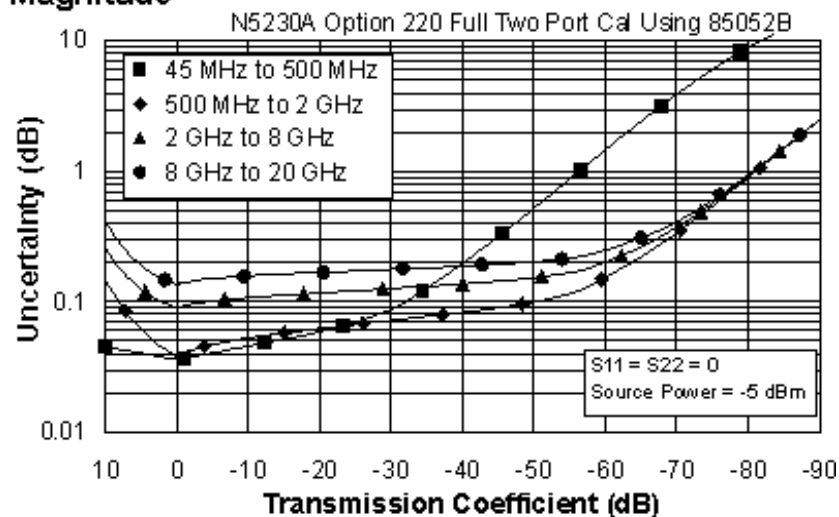


## Phase

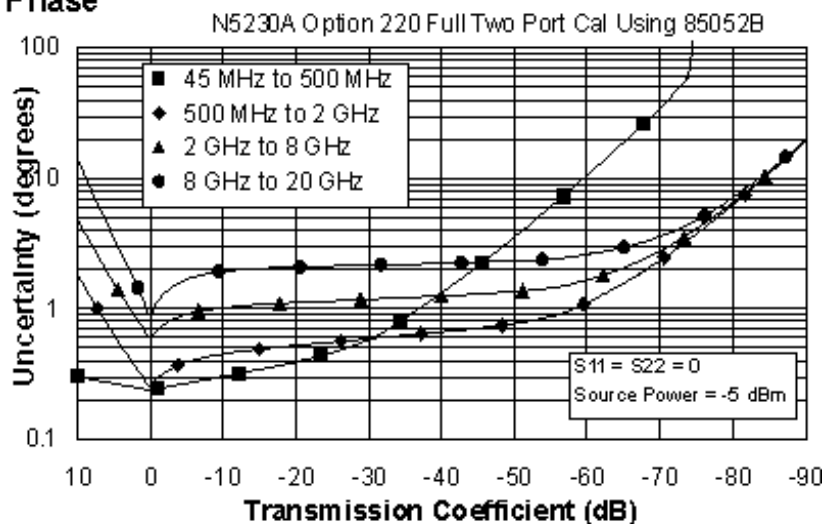


## Reflection Uncertainty (Specifications)

### Magnitude

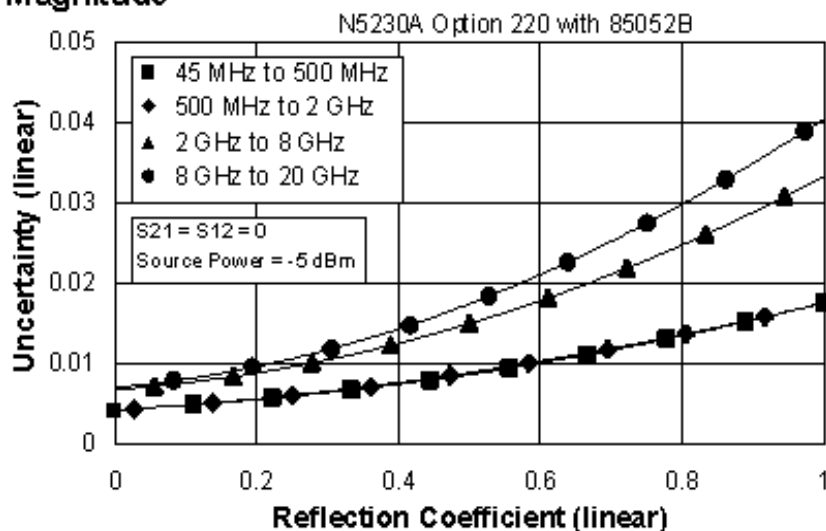

### Phase

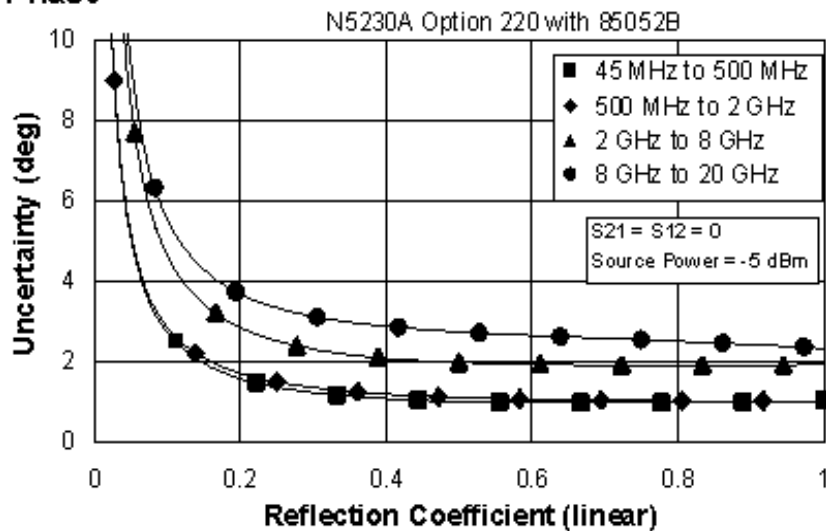

**Table 6. 85052B Calibration Kit**  
**N5230A - Option 225 (Configurable Test Set and Extended Power Range)**


Applies to the, N5230A Option 225 analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to 500 MHz  | 500 MHz to 2 GHz   | 2 to 8 GHz         | 8 to 20 GHz        |
| Directivity           | 48                 | 48                 | 44                 | 44                 |
| Source Match          | 40                 | 40                 | 33                 | 31                 |
| Load Match            | 48                 | 48                 | 44                 | 44                 |
| Reflection Tracking   | ±0.003<br>+0.02/°C | ±0.003<br>+0.02/°C | ±0.003<br>+0.03/°C | ±0.006<br>+0.03/°C |
| Transmission Tracking | ±0.010<br>+0.02/°C | ±0.014<br>+0.02/°C | ±0.062<br>+0.03/°C | ±0.104<br>+0.03/°C |


**Transmission Uncertainty (Specifications)**

**Magnitude**

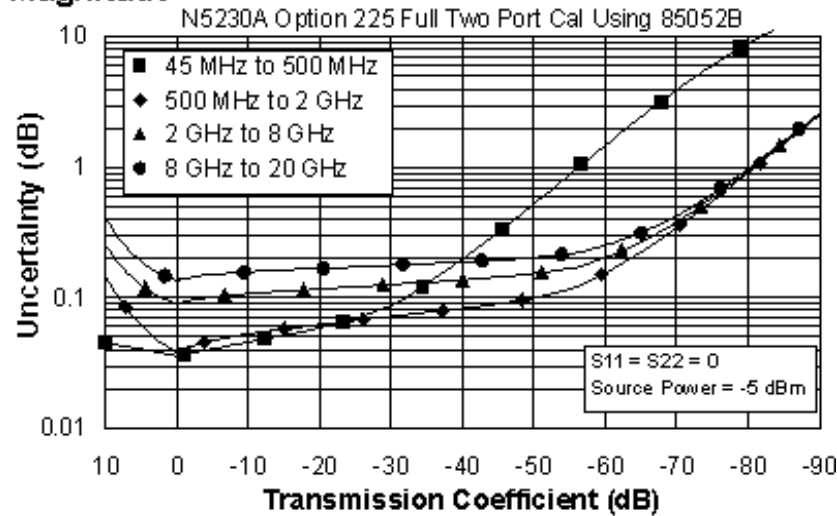

## Phase


N5230A Option 225 Full Two Port Cal Using 85052B

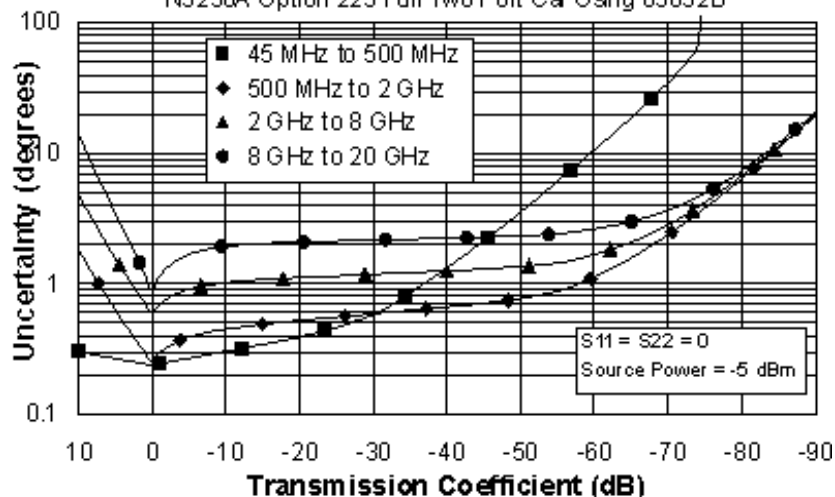

## Reflection Uncertainty (Specifications)


### Magnitude

N5230A Option 225 with 85052B

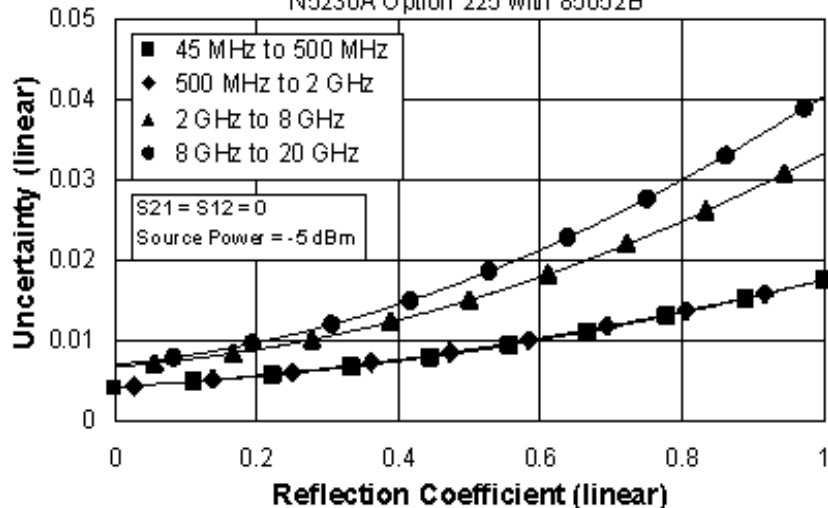

### Phase

N5230A Option 225 with 85052B

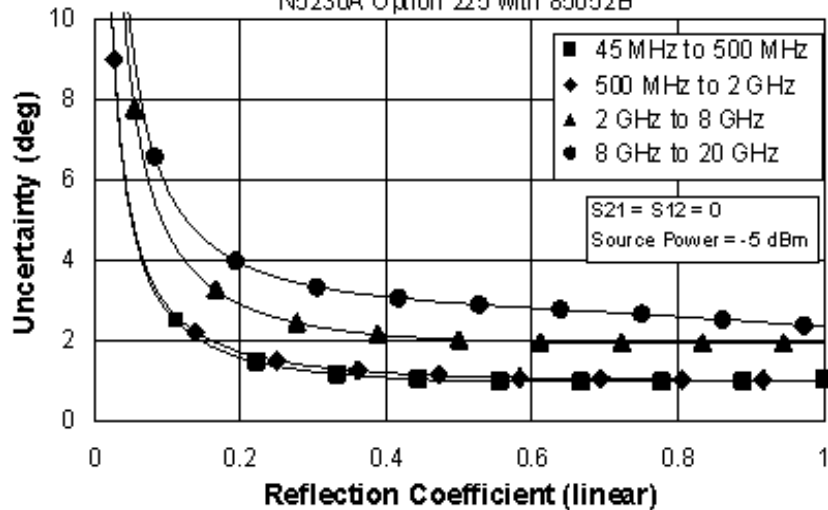



**Table 7. N4691A Electronic Calibration Module  
N5230A - Option 220 (Standard Test Set and Standard Power Range)**


Applies to the, N5230A Option 220 analyzers, N4691A (3.5mm) electronic calibration module, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to 500 MHz  | 500 MHz to 2 GHz   | 2 to 8 GHz         | 8 to 20 GHz        |
| Directivity           | 56                 | 56                 | 54                 | 49                 |
| Source Match          | 47                 | 47                 | 45                 | 44                 |
| Load Match            | 46                 | 46                 | 45                 | 43                 |
| Reflection Tracking   | ±0.050<br>+0.02/°C | ±0.050<br>+0.02/°C | ±0.070<br>+0.03/°C | ±0.090<br>+0.03/°C |
| Transmission Tracking | ±0.054<br>+0.02/°C | ±0.056<br>+0.02/°C | ±0.057<br>+0.03/°C | ±0.070<br>+0.03/°C |

**Transmission Uncertainty (Specifications)**

**Magnitude**

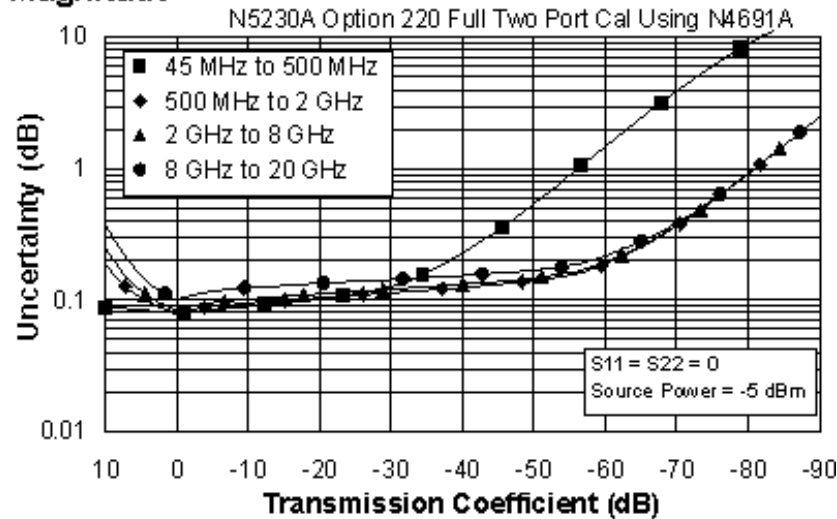


## Phase

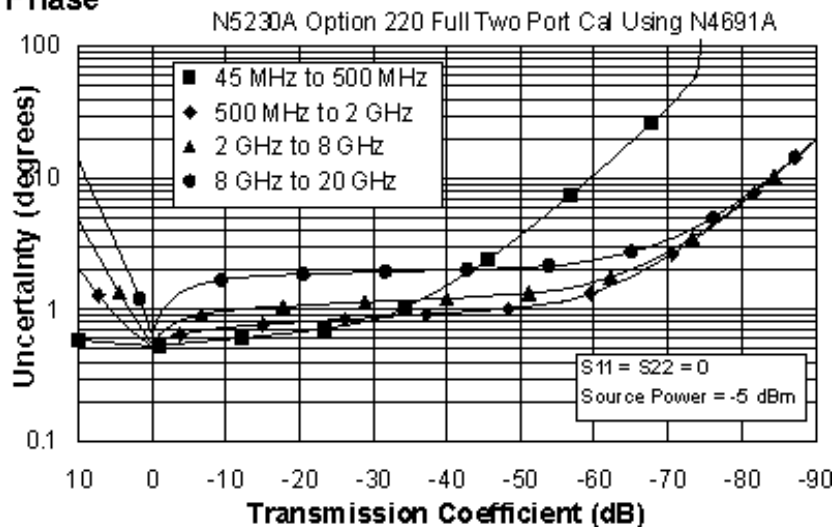


## Reflection Uncertainty (Specifications)

### Magnitude

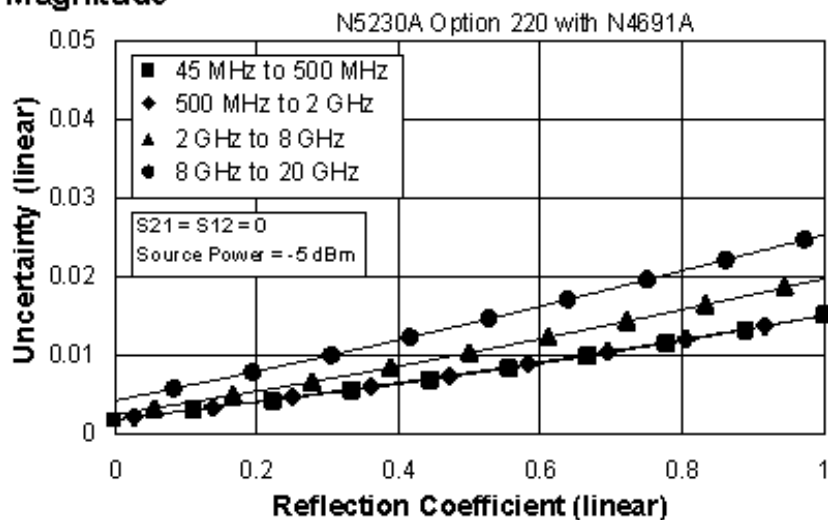

### Phase

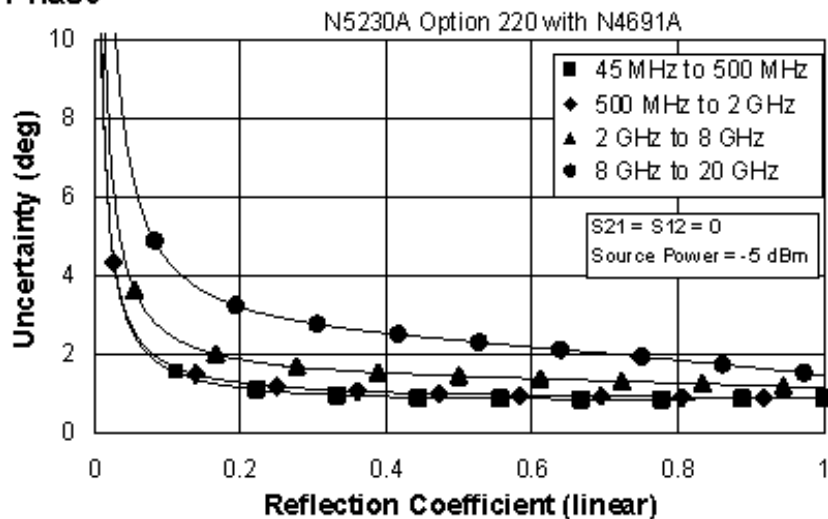

**Table 8. N4691A Electronic Calibration Module  
N5230A - Option 225 (Configurable Test Set and Extended Power Range)**


Applies to the, N5230A Option 225 analyzers, N4691A Electronic Calibration Module, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |                    |                    |
|-----------------------|--------------------|--------------------|--------------------|--------------------|
|                       | 45 MHz to 500 MHz  | 500 MHz to 2 GHz   | 2 to 8 GHz         | 8 to 20 GHz        |
| Directivity           | 56                 | 56                 | 54                 | 49                 |
| Source Match          | 47                 | 47                 | 45                 | 44                 |
| Load Match            | 46                 | 46                 | 45                 | 43                 |
| Reflection Tracking   | ±0.050<br>+0.02/°C | ±0.050<br>+0.02/°C | ±0.070<br>+0.03/°C | ±0.090<br>+0.03/°C |
| Transmission Tracking | ±0.054<br>+0.02/°C | ±0.056<br>+0.02/°C | ±0.057<br>+0.03/°C | ±0.070<br>+0.03/°C |

**Transmission Uncertainty (Specifications)**

**Magnitude**

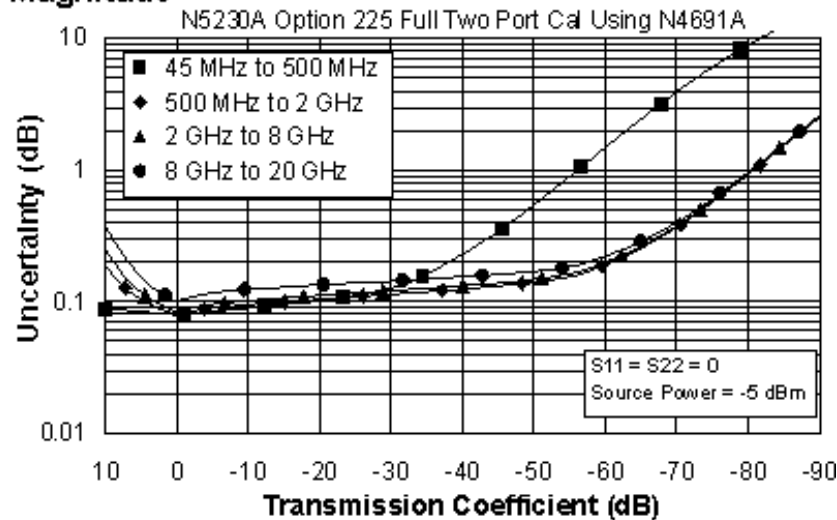


## Phase

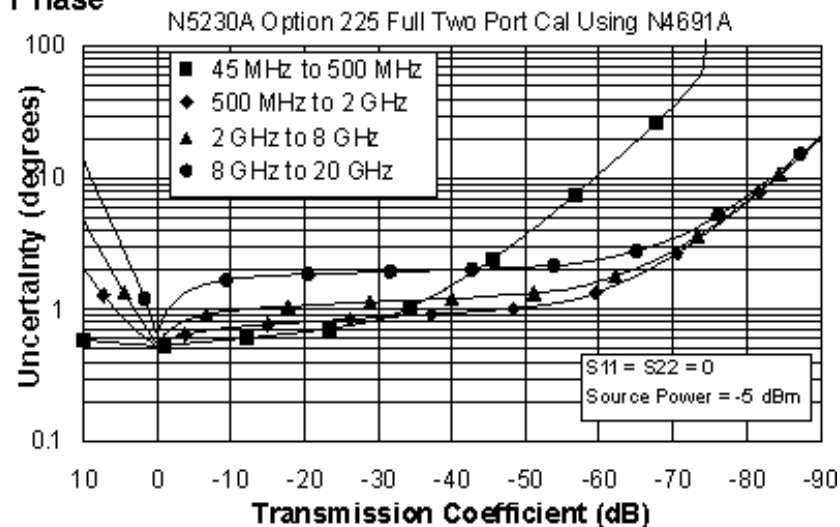


## Reflection Uncertainty (Specifications)

### Magnitude

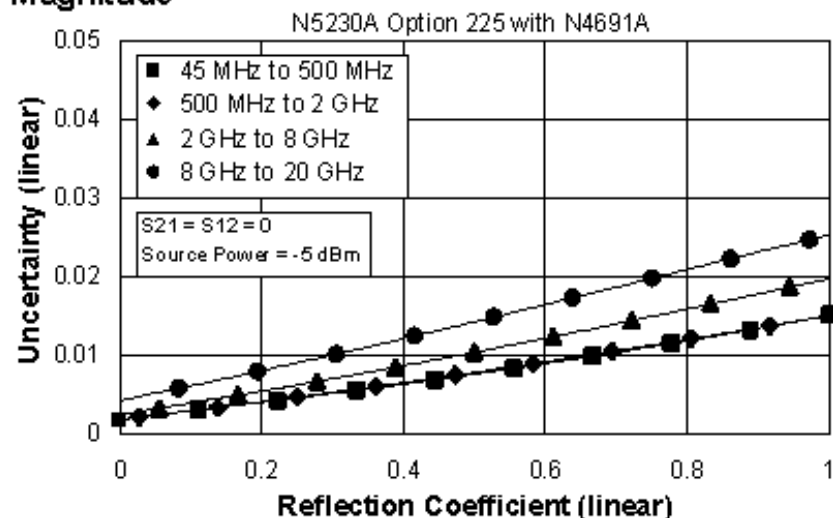

### Phase

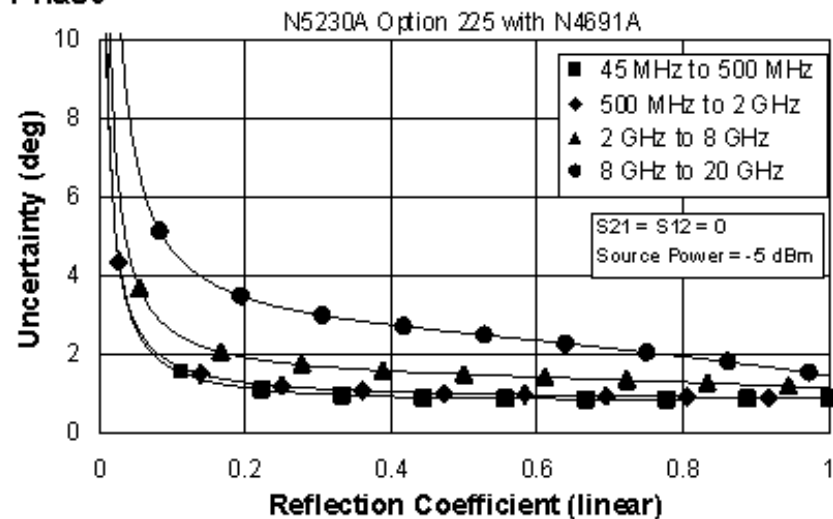

This N5230A document does not present specifications for the 85052C or 85052D Calibration Kit. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the data and curves for the 85052C or the 85052D Calibration Kit or your PNA setup. View the equations used to generate the uncertainty curves.

## N5230A Corrected System Performance with 3.5mm Connectors<sup>1</sup>

### Options 240/245

<sup>1</sup> From 300 kHz to 10 MHz, performance is characterized as "typical". To generate these typical values, please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator).

### 85052B Calibration Kit

#### N5230A - Option 240 - Standard Test Set and Standard Power Range

#### N5230A Option 245 - Configurable Test Set and Extended Power Range

### N4691A Electronic Calibration (ECal) Module

#### N5230A - Option 240 - Standard Test Set and Standard Power Range

#### N5230A Option 245 - Configurable Test Set and Extended Power Range

**Note:** For any  $S_{ij}$  reflection measurement:

- $S_{jj} = 0$ .

For any  $S_{ij}$  transmission measurement:

- $S_{ji} = S_{ij}$  when  $S_{ij} \leq 1$
- $S_{ji} = 1/S_{ij}$  when  $S_{ij} \geq 1$
- $S_{kk} = 0$  for all  $k$

### Table 3. 85052B Calibration Kit

#### N5230A - Option 240 (Standard Test Set and Standard Power Range)


Applies to the, N5230A Option 240 analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^\circ \pm 3^\circ \text{C}$ , with  $< 1^\circ \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                     |                                        |                                        |                                        |
|-----------------------|----------------------------------------|----------------------------------------|----------------------------------------|----------------------------------------|
|                       | 10 MHz to<br>500 MHz                   | 500 MHz to<br>2 GHz                    | 2 to<br>8 GHz                          | 8 to<br>20 GHz                         |
| Directivity           | 48                                     | 48                                     | 44                                     | 44                                     |
| Source Match          | 40                                     | 40                                     | 33                                     | 31                                     |
| Load Match            | 48                                     | 48                                     | 44                                     | 44                                     |
| Reflection Tracking   | $\pm 0.003$<br>$+0.010/^\circ\text{C}$ | $\pm 0.003$<br>$+0.010/^\circ\text{C}$ | $\pm 0.003$<br>$+0.020/^\circ\text{C}$ | $\pm 0.006$<br>$+0.030/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.017$<br>$+0.010/^\circ\text{C}$ | $\pm 0.017$<br>$+0.010/^\circ\text{C}$ | $\pm 0.062$<br>$+0.020/^\circ\text{C}$ | $\pm 0.125$<br>$+0.030/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

## Magnitude

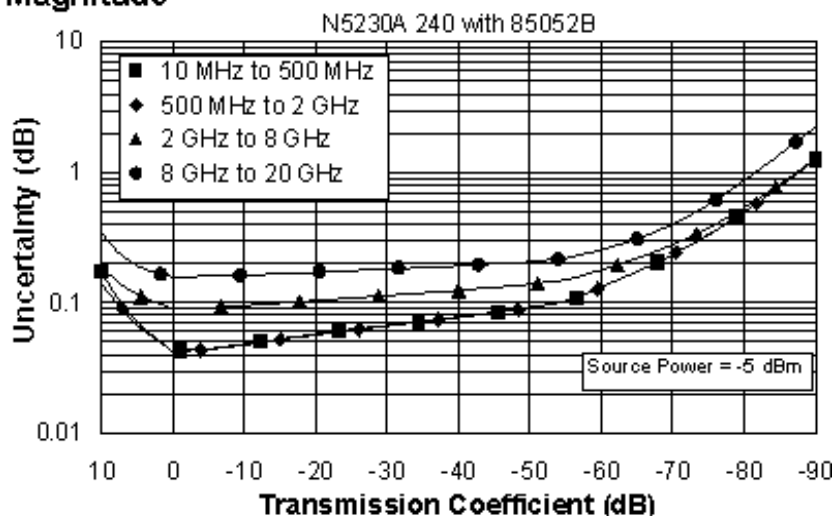


## Phase

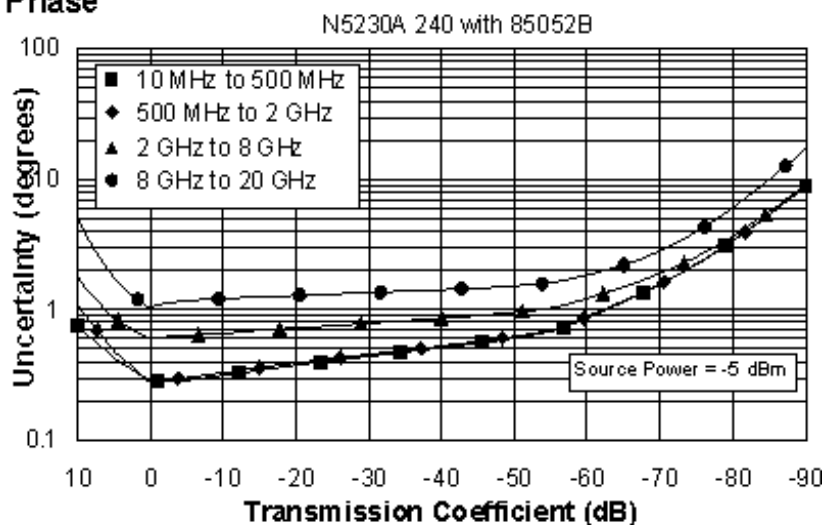


## Reflection Uncertainty (Specifications)

### Magnitude

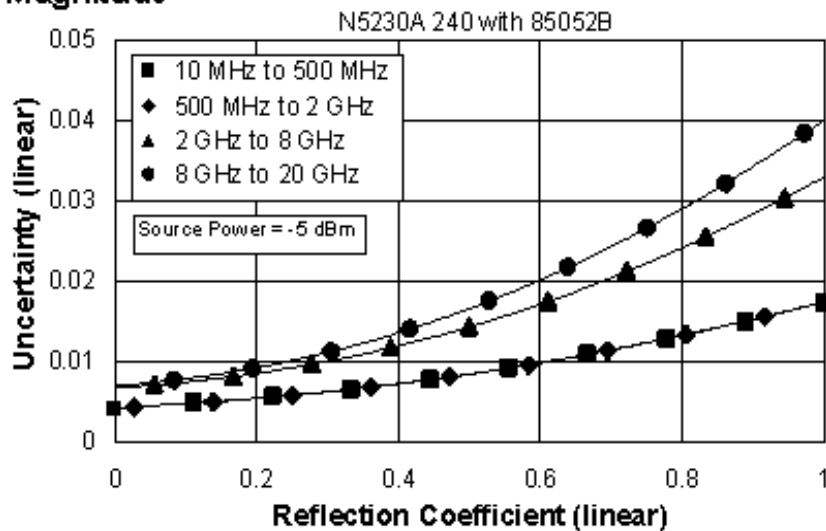

## Phase

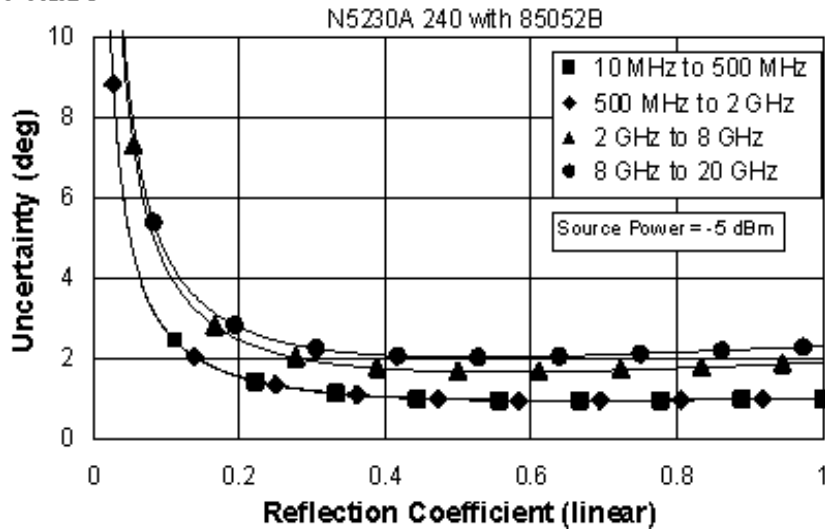

**Table 4.** 85052B Calibration Kit

### N5230A - Option 245 (Configurable Test Set and Extended Power Range)

Applies to the, N5230A Option 245 analyzers, 85052B (3.5mm) calibration kit, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:


Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB)  |                     |                     |                     |
|-----------------------|---------------------|---------------------|---------------------|---------------------|
|                       | 10 MHz to 500 MHz   | 500 MHz to 2 GHz    | 2 to 8 GHz          | 8 to 20 GHz         |
| Directivity           | 48                  | 48                  | 44                  | 44                  |
| Source Match          | 40                  | 40                  | 33                  | 31                  |
| Load Match            | 48                  | 48                  | 44                  | 44                  |
| Reflection Tracking   | ±0.003<br>+0.010/°C | ±0.003<br>+0.010/°C | ±0.003<br>+0.020/°C | ±0.006<br>+0.030/°C |
| Transmission Tracking | ±0.017<br>+0.010/°C | ±0.017<br>+0.010/°C | ±0.062<br>+0.020/°C | ±0.125<br>+0.030/°C |


## Transmission Uncertainty (Specifications)



## Magnitude

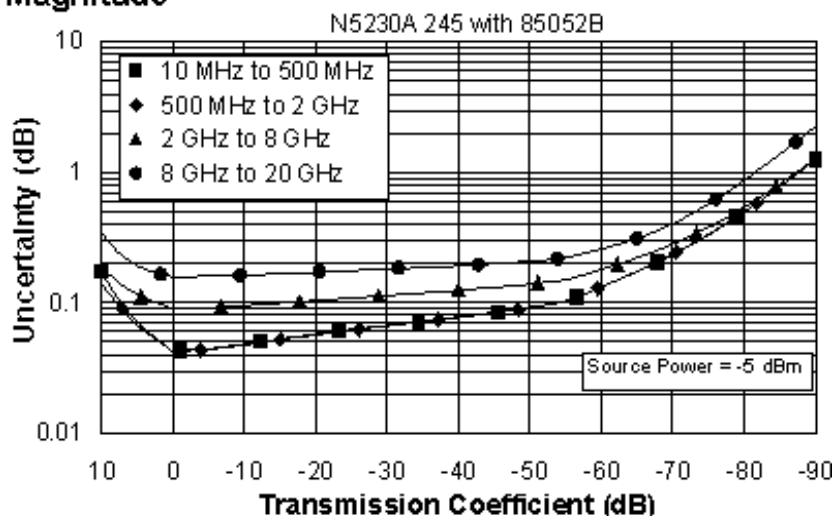


## Phase

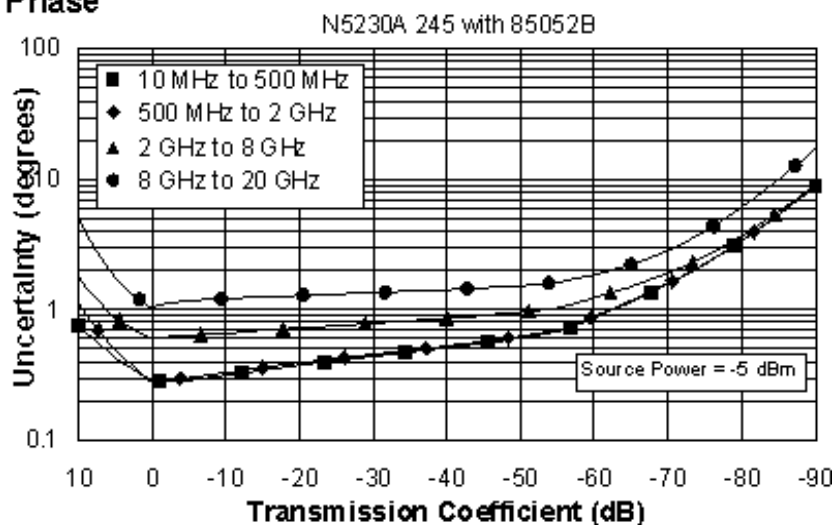


## Reflection Uncertainty (Specifications)

### Magnitude

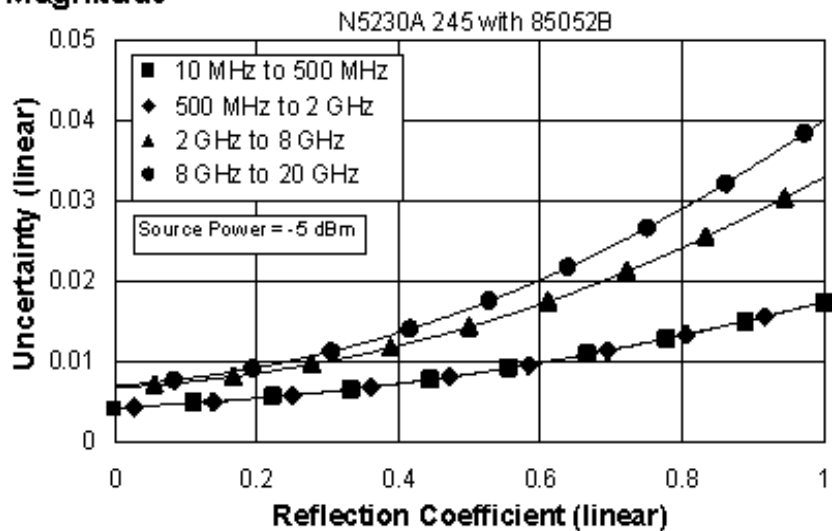

## Phase

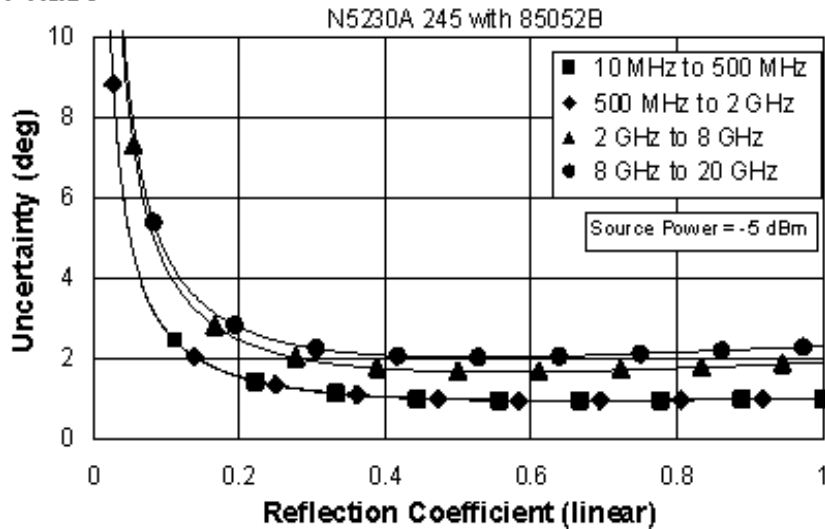

**Table 5.** N4691A Electronic Calibration Module  
N5230A - Option 240 (Standard Test Set and Standard Power Range)


Applies to the, N5230A Option 240 analyzers, N4691A (3.5mm) electronic calibration module, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                       |                                          |                                          |                                          |
|-----------------------|------------------------------------------|------------------------------------------|------------------------------------------|------------------------------------------|
|                       | 45 MHz to<br>500 MHz                     | 500 MHz to<br>2 GHz                      | 2 to<br>8 GHz                            | 8 to<br>20 GHz                           |
| Directivity           | 56                                       | 56                                       | 54                                       | 49                                       |
| Source Match          | 47                                       | 47                                       | 45                                       | 44                                       |
| Load Match            | 46                                       | 46                                       | 45                                       | 43                                       |
| Reflection Tracking   | $\pm 0.050$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.050$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.070$<br>$+0.020/^{\circ}\text{C}$ | $\pm 0.090$<br>$+0.030/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.055$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.056$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.057$<br>$+0.020/^{\circ}\text{C}$ | $\pm 0.071$<br>$+0.030/^{\circ}\text{C}$ |

## Transmission Uncertainty (Specifications)

## Magnitude

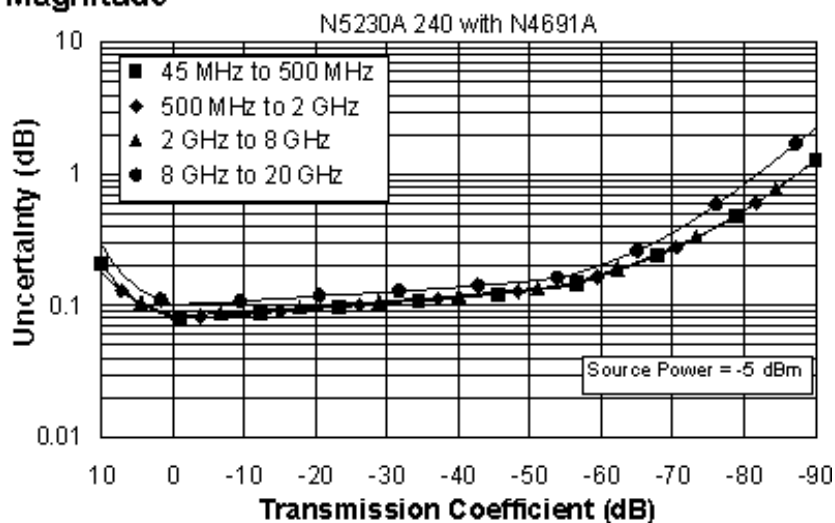


## Phase

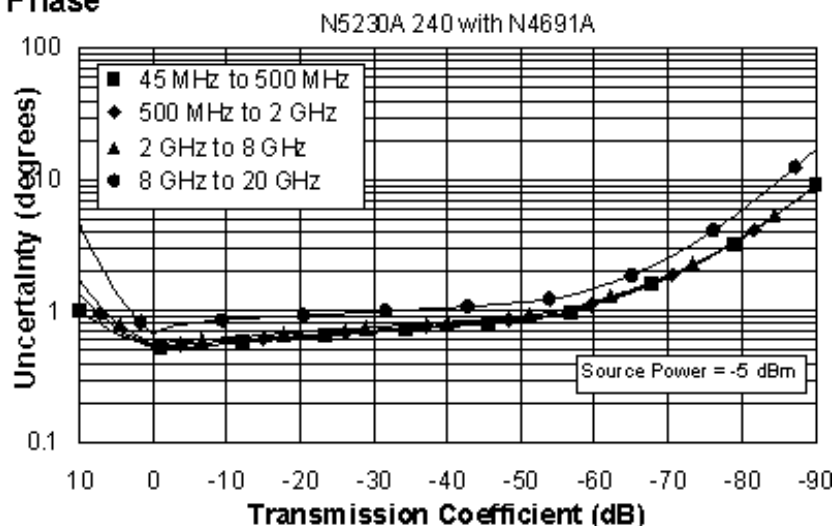


## Reflection Uncertainty (Specifications)

### Magnitude

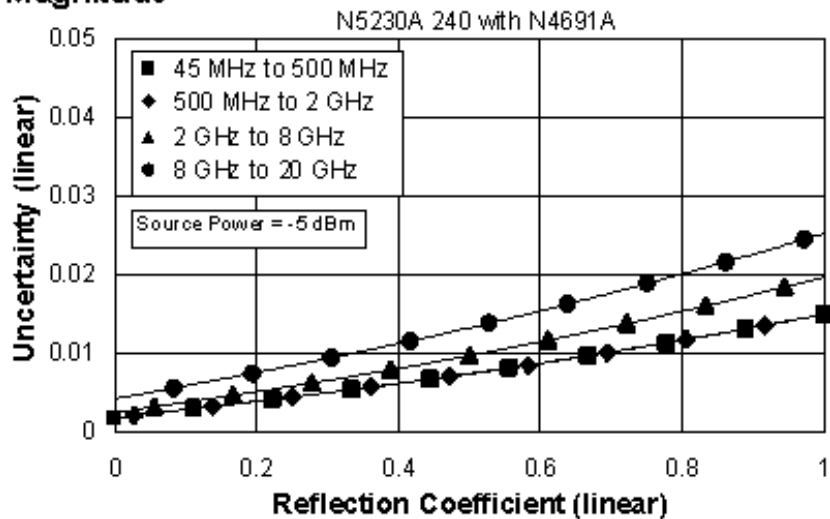

## Phase

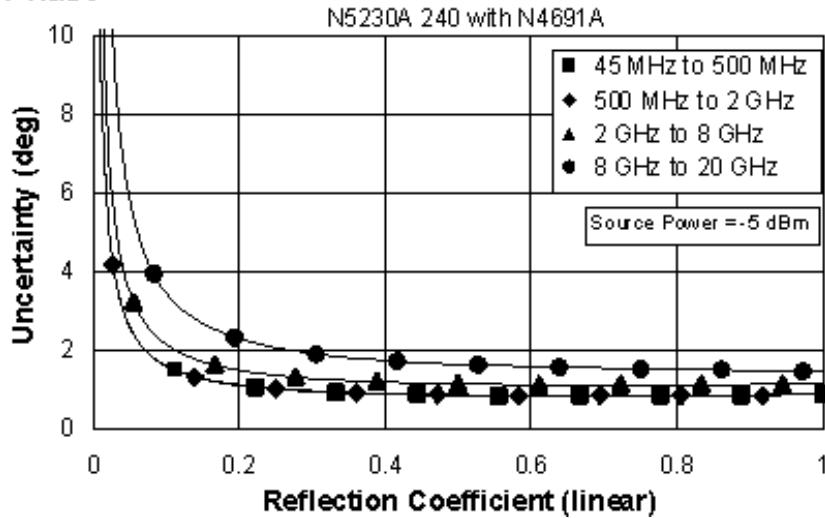

**Table 6.** N4691A Electronic Calibration Module  
N5230A - Option 245 (Configurable Test Set and Extended Power Range)


Applies to the, N5230A Option 245 analyzers, N4691A (3.5 mm) Electronic Calibration Module, 85131F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                       |                                          |                                          |                                          |
|-----------------------|------------------------------------------|------------------------------------------|------------------------------------------|------------------------------------------|
|                       | 45 MHz to<br>500 MHz                     | 500 MHz to<br>2 GHz                      | 2 to<br>8 GHz                            | 8 to<br>20 GHz                           |
| Directivity           | 56                                       | 56                                       | 54                                       | 49                                       |
| Source Match          | 47                                       | 47                                       | 45                                       | 44                                       |
| Load Match            | 46                                       | 46                                       | 45                                       | 43                                       |
| Reflection Tracking   | $\pm 0.050$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.050$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.070$<br>$+0.020/^{\circ}\text{C}$ | $\pm 0.090$<br>$+0.030/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.055$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.056$<br>$+0.010/^{\circ}\text{C}$ | $\pm 0.057$<br>$+0.020/^{\circ}\text{C}$ | $\pm 0.071$<br>$+0.030/^{\circ}\text{C}$ |

## Transmission Uncertainty (Specifications)

## Magnitude

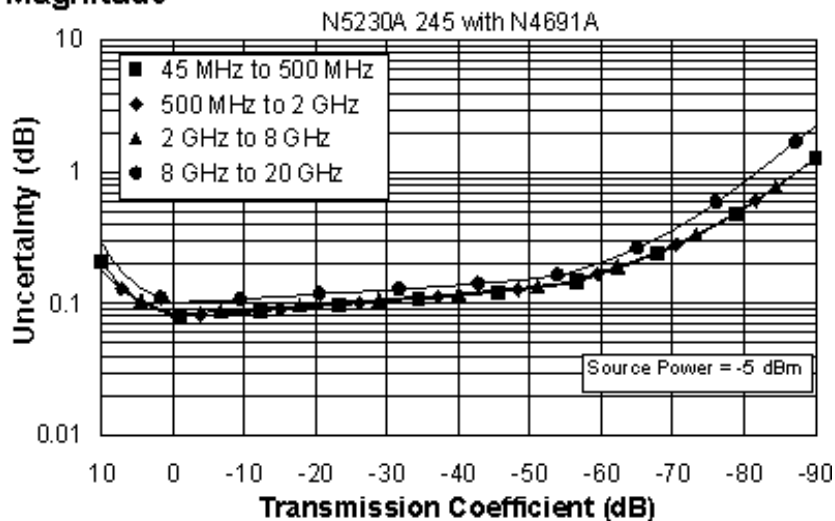


## Phase

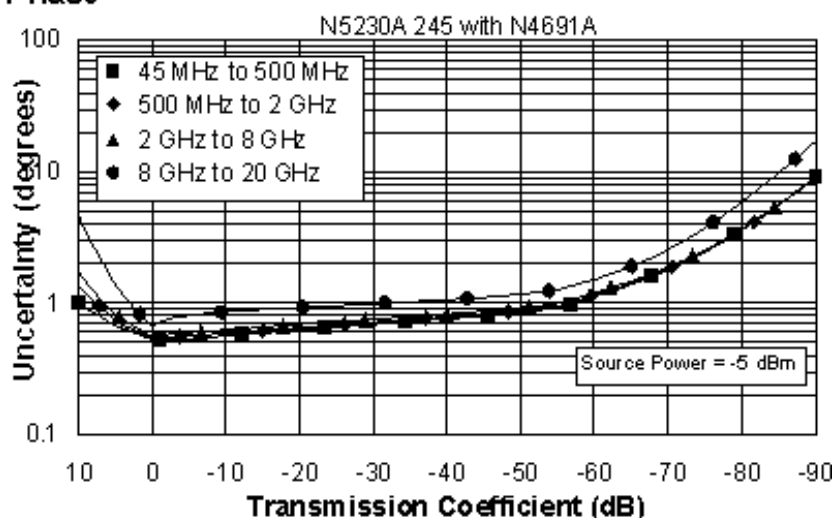


## Reflection Uncertainty (Specifications)

### Magnitude

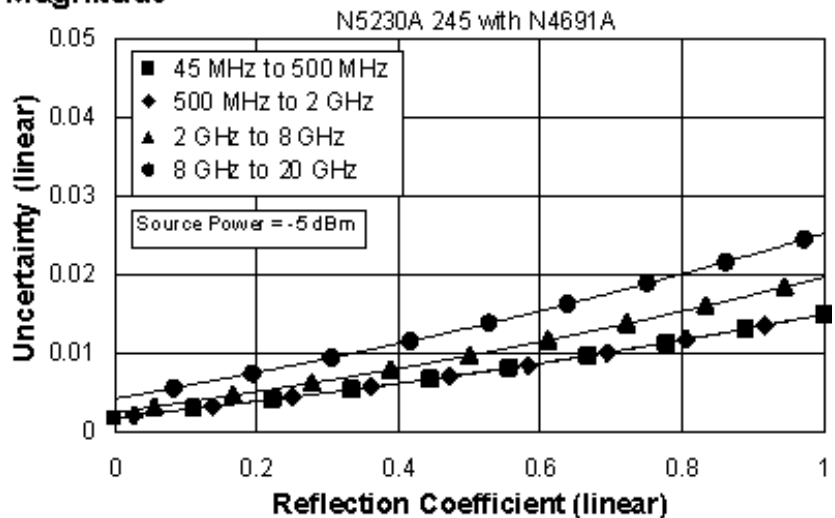

# Phase

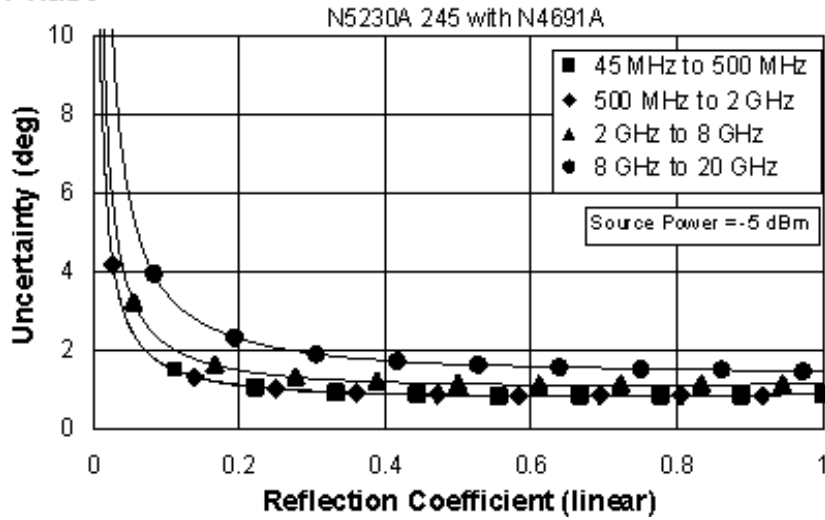

This N5230A document does not present specifications for the 85052C or 85052D Calibration Kit. Please download our free Uncertainty Calculator from [http://www.agilent.com/find/na\\_calculator](http://www.agilent.com/find/na_calculator) to generate the data and curves for the 85052C or the 85052D Calibration Kit. View the [equations](#) used to generate the uncertainty curves.

## E8363/4B Corrected System Performance with WR-42 Connectors

### K11644A Calibration Kit:

#### Standard Configuration and Standard Power Range (E8363/4B)


#### Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

**Table 27.** K11644A Calibration Kit  
Standard Configuration and Standard Power Range  
(E8363/4B)


Applies to the, E8363/4B analyzers, K11644A (WR-42) calibration kit, 85134F flexible test port cable set with the K281C launch set,, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|
|                       | 18 to 20 GHz                            | 20 to 26.5 GHz                          |
| Directivity           | 50                                      | 50                                      |
| Source Match          | 50                                      | 50                                      |
| Load Match            | 50                                      | 50                                      |
| Reflection Tracking   | $\pm 0.000$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.000$<br>$+0.02/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.014$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.018$<br>$+0.02/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications) Magnitude

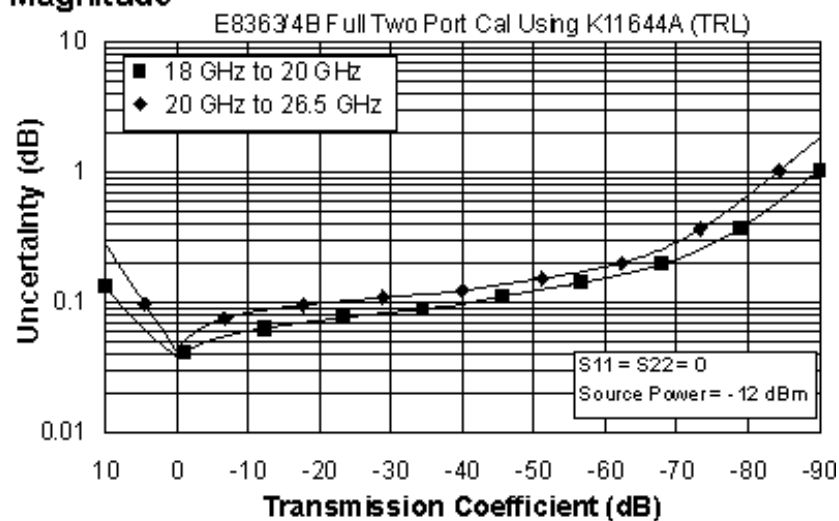


### Phase

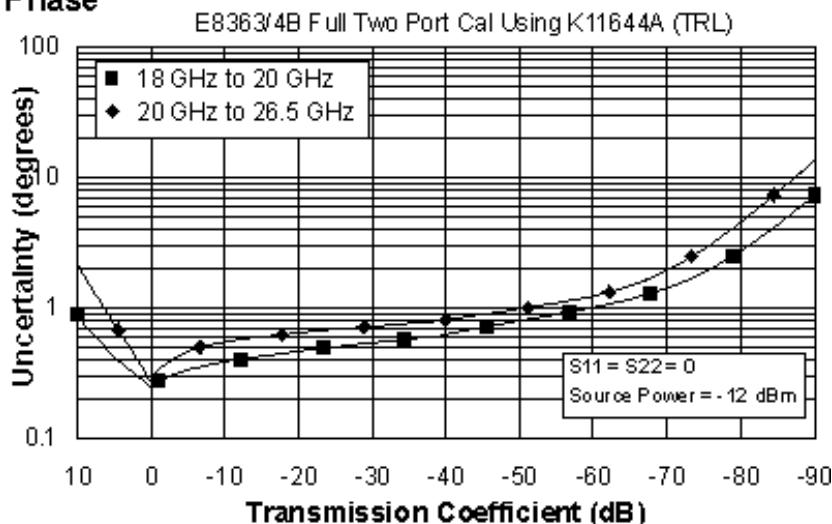

### Reflection Uncertainty (Specifications)

#### Magnitude

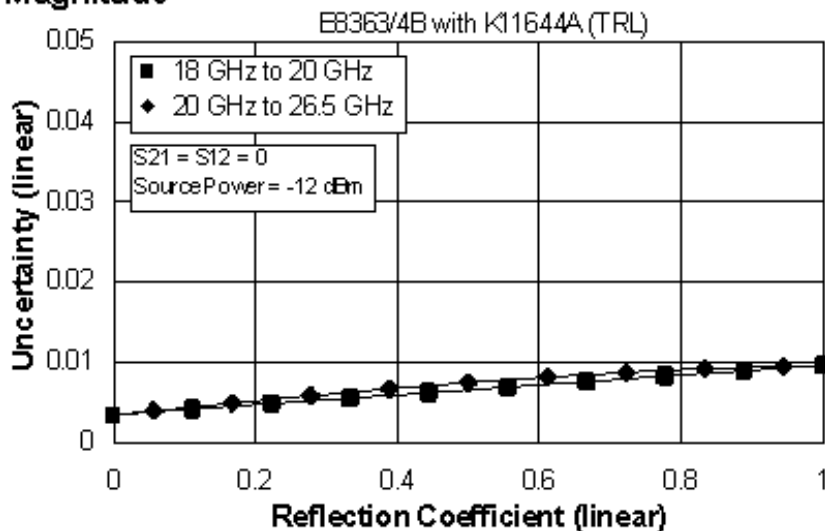

#### Phase

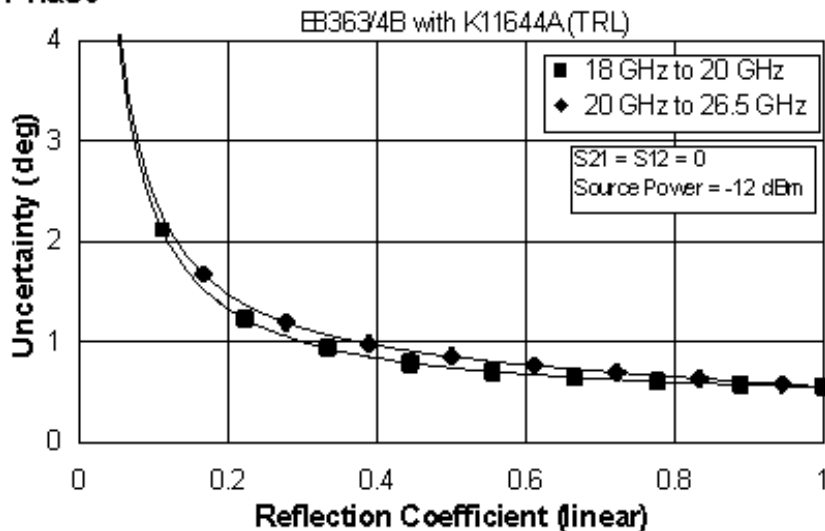


Table 28. K11644A Calibration Kit



## Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E8363/4B analyzers, K11644A (WR-42) calibration kit, 85134F flexible test port cable set with the K281C launch set., and a full 2-port calibration. Also applies to the following condition:

Environmental temperature  $23 \pm 3$  °C, with  $< 1$  °C deviation from calibration temperature


| Description           | Specification (dB)                    |                                       |
|-----------------------|---------------------------------------|---------------------------------------|
|                       | 18 to 20 GHz                          | 20 to 26.5 GHz                        |
| Directivity           | 50                                    | 50                                    |
| Source Match          | 50                                    | 50                                    |
| Load Match            | 50                                    | 50                                    |
| Reflection Tracking   | $\pm 0.000$<br>$+0.02/^\circ\text{C}$ | $\pm 0.000$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.016$<br>$+0.02/^\circ\text{C}$ | $\pm 0.019$<br>$+0.02/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

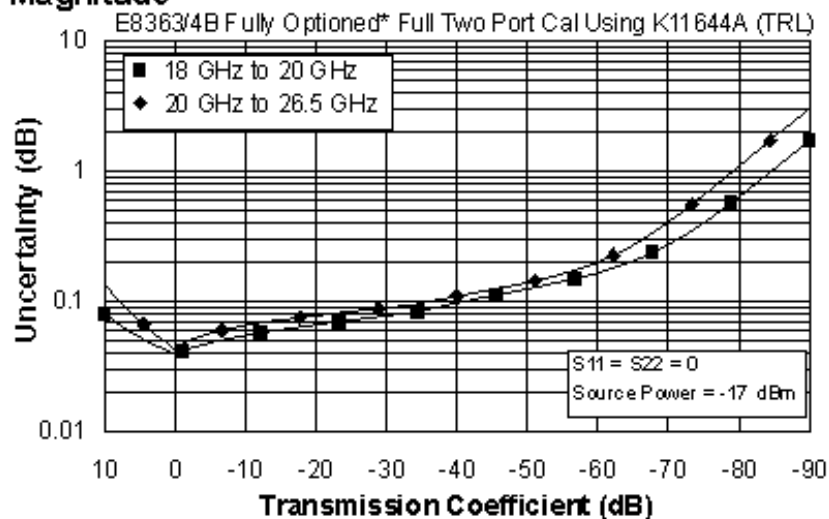


### Phase

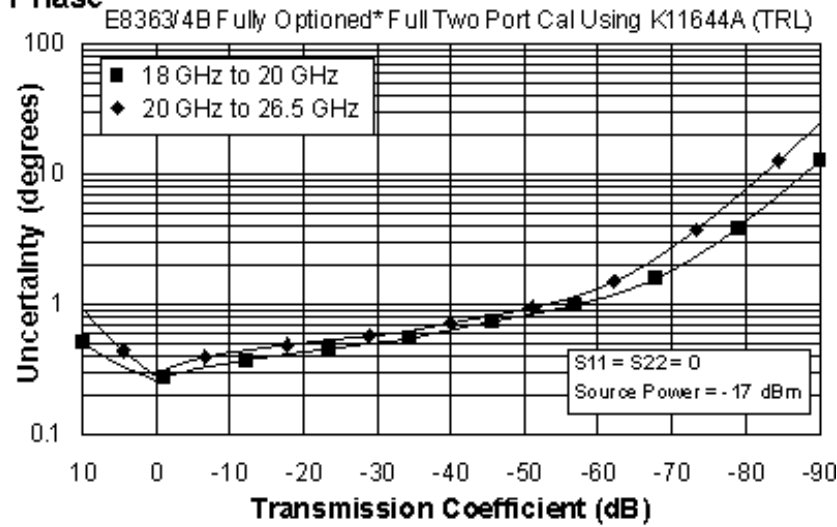


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

### Reflection Uncertainty (Specifications) Magnitude

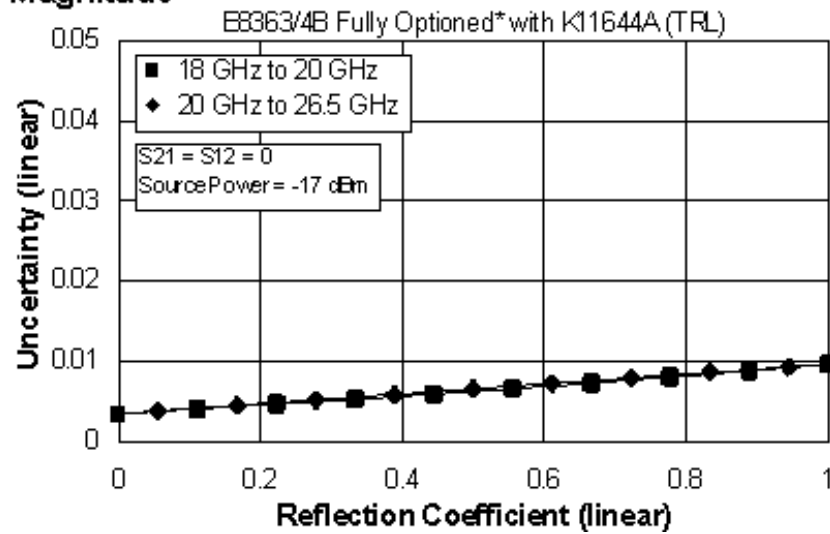

### Phase

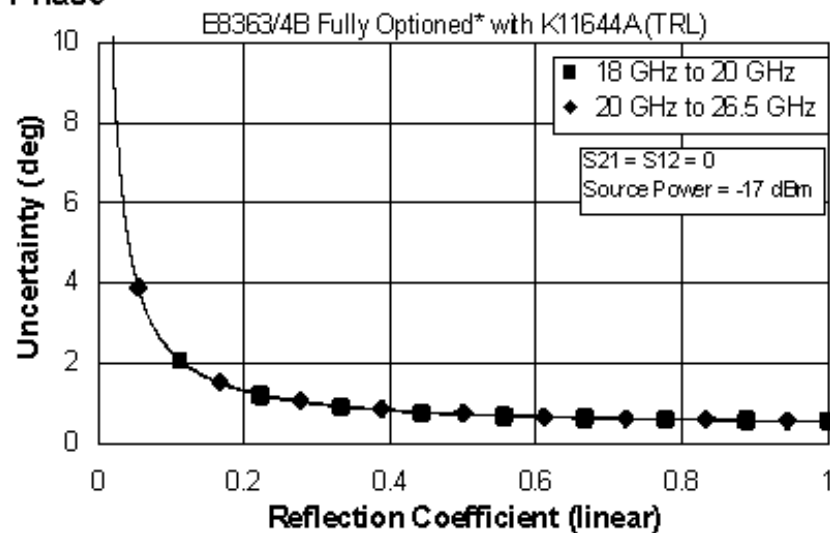

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## E836xB Corrected System Performance with WR-62 Connectors

### P11644A Calibration Kit:

#### Standard Configuration and Standard Power Range (E836xB)


#### Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

**Table 29.** P11644A Calibration Kit  
Standard Configuration and Standard Power Range  
(E836xB)


Applies to the, E836xB analyzers, P11644A (WR-62) calibration kit, 85132F flexible test port cable set with the P281B and P281C launch sets, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |
|-----------------------|-----------------------------------------|
|                       | <b>12.4 to<br/>18 GHz</b>               |
| Directivity           | 50                                      |
| Source Match          | 50                                      |
| Load Match            | 50                                      |
| Reflection Tracking   | $\pm 0.000$<br>$+0.02/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.014$<br>$+0.02/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications) Magnitude

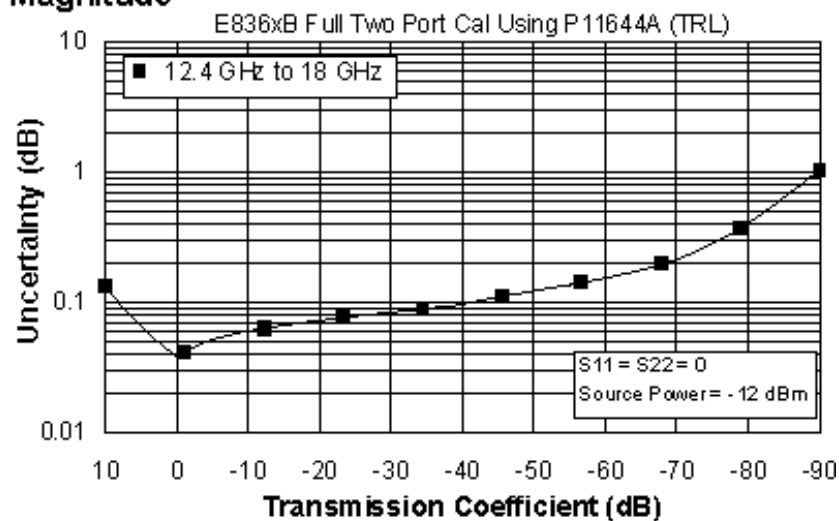


### Phase

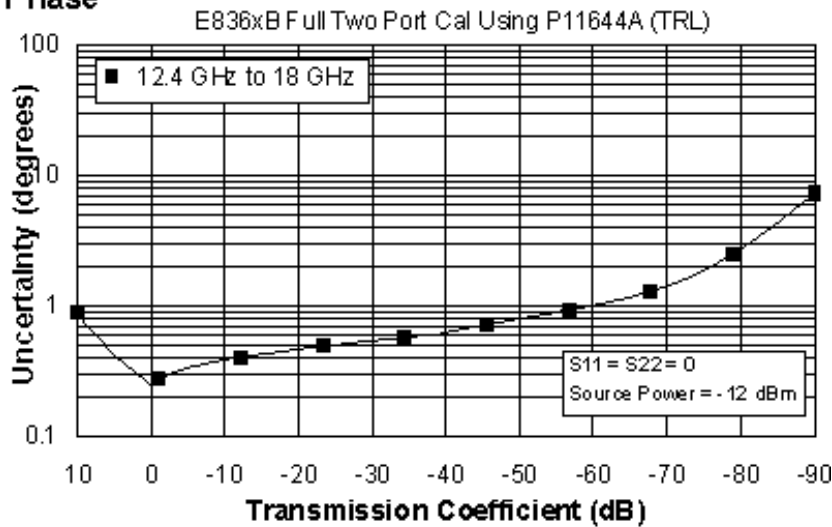

### Reflection Uncertainty (Specifications)

#### Magnitude

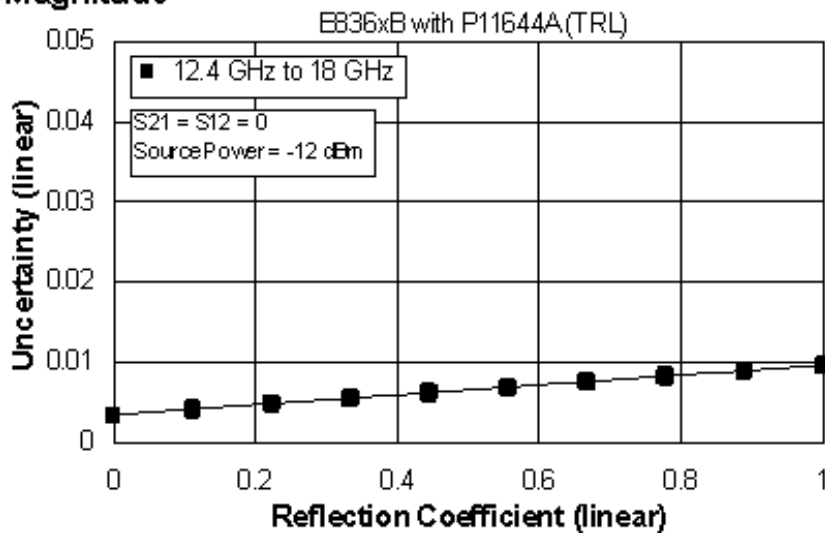

#### Phase

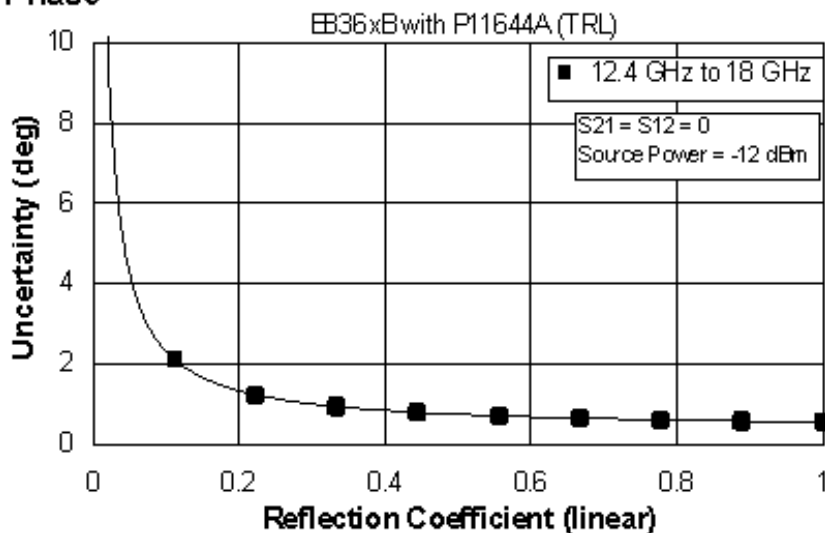


Table 30. P11644A Calibration Kit

## Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)


Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E836xB analyzers, P11644A (WR-62) calibration kit, 85132F flexible test port cable set with the P281B and P281C launch sets, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23 \pm 3 \text{ }^\circ\text{C}$ , with  $< 1 \text{ }^\circ\text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                    |
|-----------------------|---------------------------------------|
|                       |                                       |
| Directivity           | 50                                    |
| Source Match          | 50                                    |
| Load Match            | 50                                    |
| Reflection Tracking   | $\pm 0.000$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.016$<br>$+0.02/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

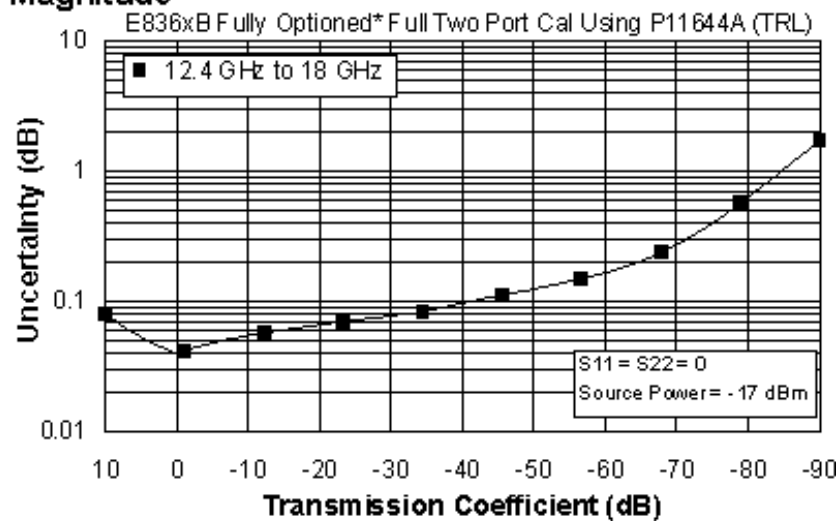


### Phase

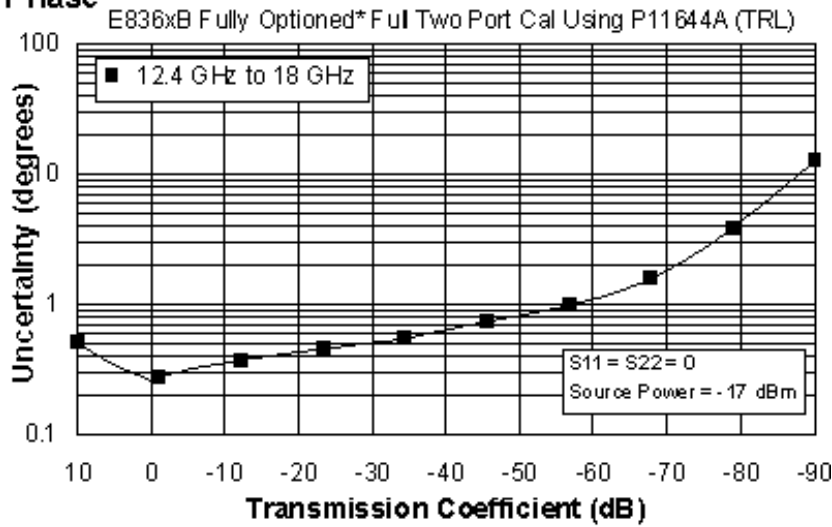


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

### Reflection Uncertainty (Specifications)

#### Magnitude

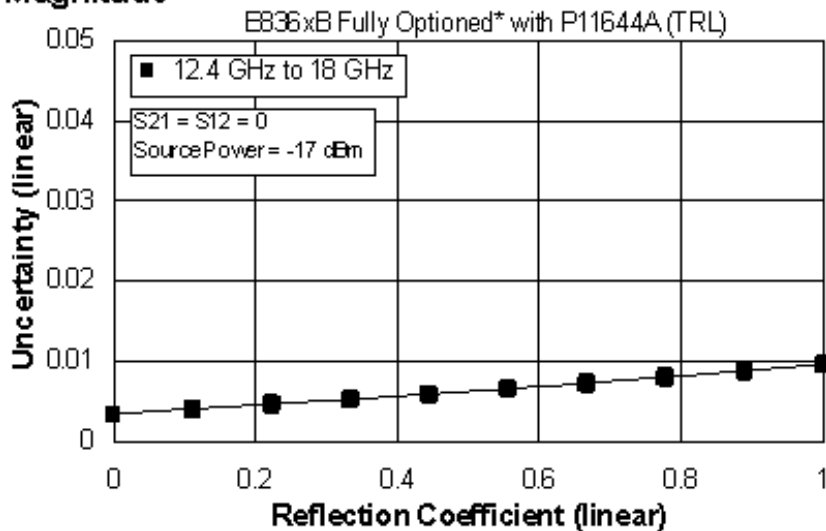

### Phase

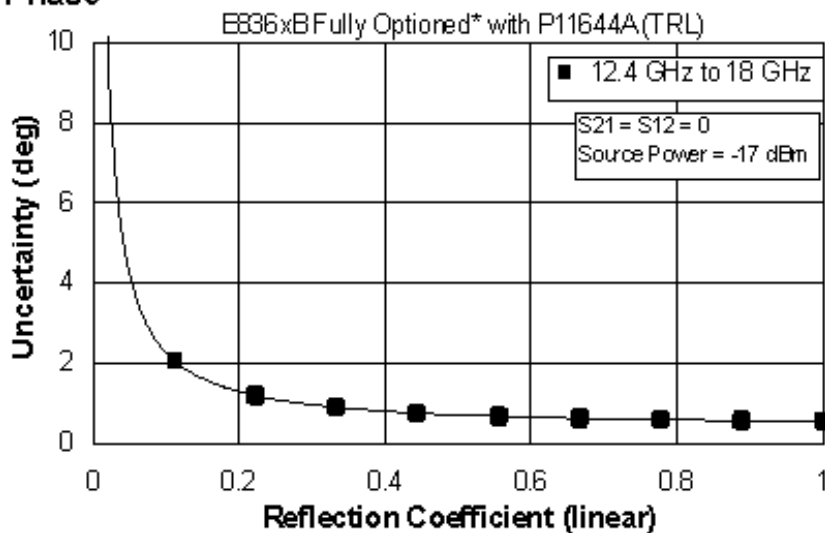

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)



## E836xB Corrected System Performance with 7mm Connectors

---

### 85050B Calibration Kit:

**Standard Configuration and Standard Power Range (E836xB)**

**Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)**

### 85050C Calibration Kit:

**Standard Configuration and Standard Power Range (E836xB)**

**Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)**

### 85050D Calibration Kit:

**Standard Configuration and Standard Power Range (E836xB)**

**Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)**

---


**Table 15.** 85050B Calibration Kit  
Standard Configuration and Standard Power Range  
(E836xB)

Applies to the, E836xB analyzers, 85050B (7mm) calibration kit, 85132F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB) |                    |
|-----------------------|--------------------|--------------------|
|                       | 0.045 to<br>2 GHz  | 2 to<br>18 GHz     |
| Directivity           | 52                 | 52                 |
| Source Match          | 48                 | 41                 |
| Load Match            | 52                 | 47                 |
| Reflection Tracking   | ±0.003<br>+0.02/°C | ±0.047<br>+0.02/°C |
| Transmission Tracking | ±0.004<br>+0.02/°C | ±0.032<br>+0.02/°C |

## Transmission Uncertainty (Specifications)

### Magnitude

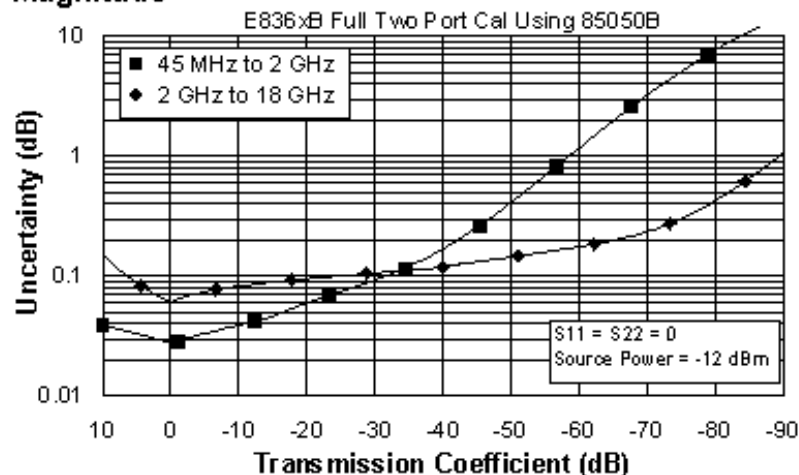


### Phase

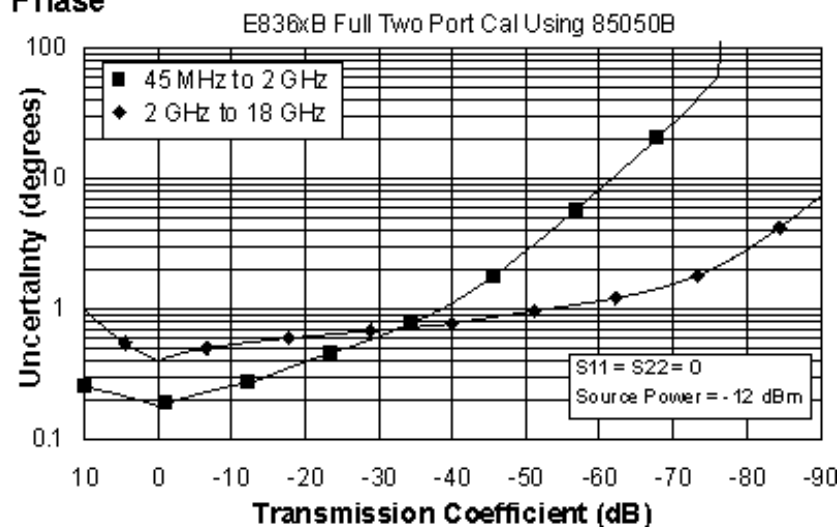


## Reflection Uncertainty (Specifications)

### Magnitude

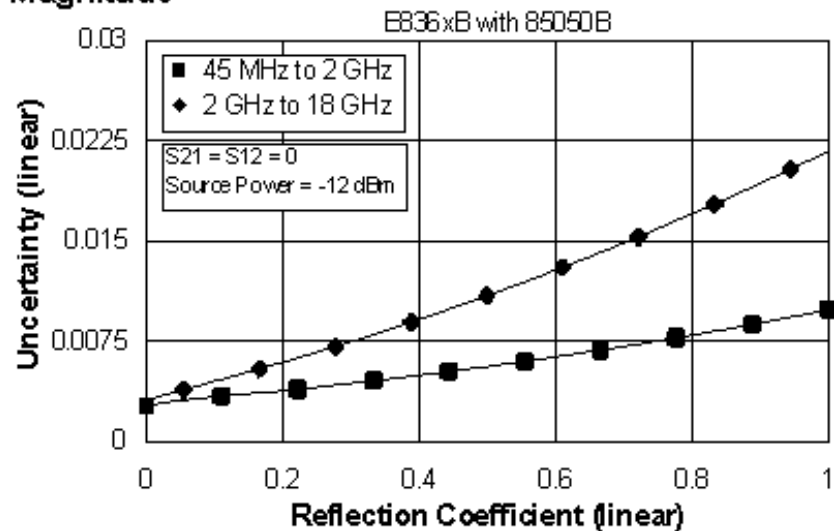

## Phase

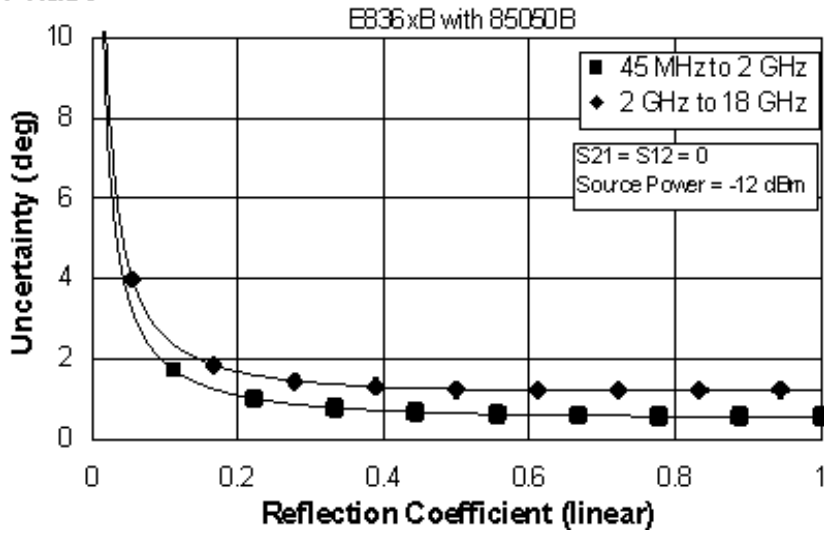

**Table 16.** 85050B Calibration Kit

Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)


Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E836xB analyzers, 85050B (7mm) calibration kit, 85132F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|
|                       | 0.045 to<br>2 GHz                       | 2 to<br>18 GHz                          |
| Directivity           | 52                                      | 52                                      |
| Source Match          | 48                                      | 41                                      |
| Load Match            | 52                                      | 47                                      |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.047$<br>$+0.02/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.008$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.034$<br>$+0.02/^{\circ}\text{C}$ |

## Transmission Uncertainty (Specifications)

## Magnitude

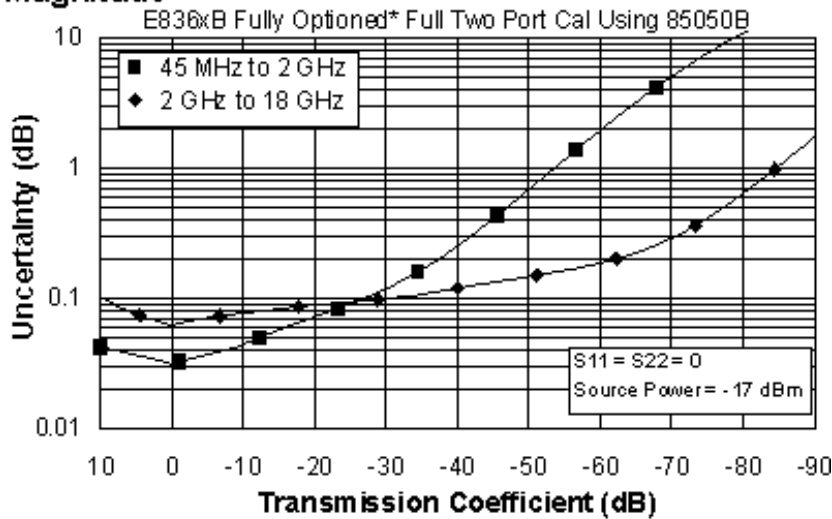


## Phase

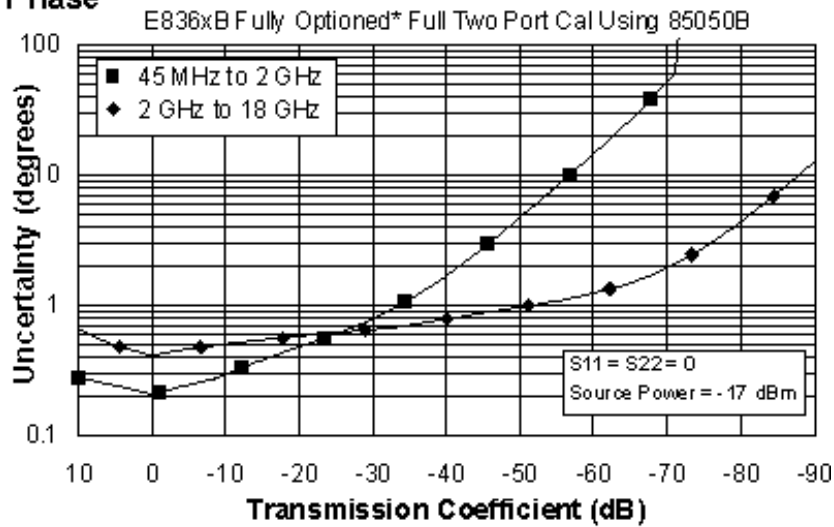


\*Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

## Magnitude

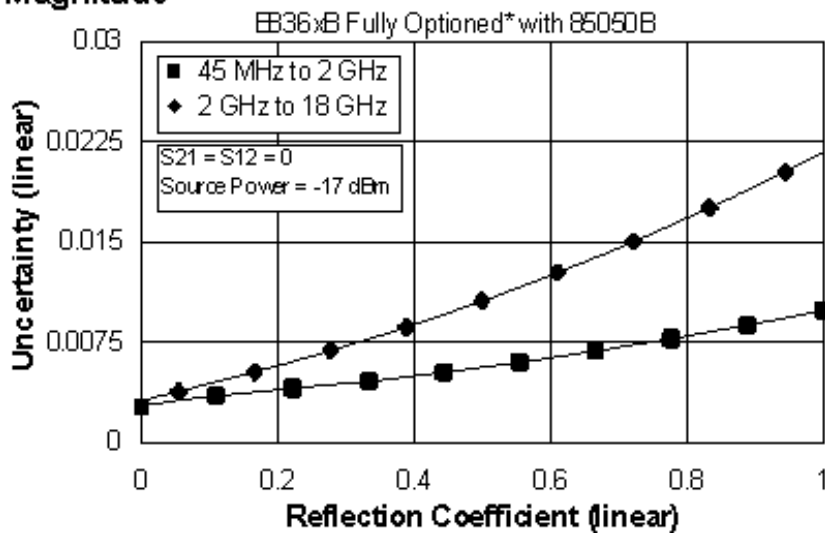

## Phase

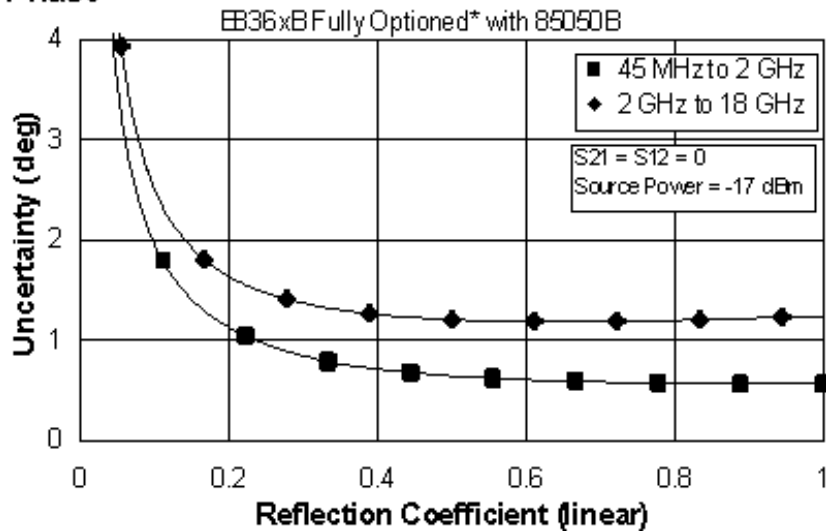

\*Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)


**Table 17.** 85050C Calibration Kit

Standard Configuration and Standard Power Range  
 (E836xB)


Applies to the, E836xB analyzers, 85050C (7mm) calibration kit, 85132F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB)                    |                                       |
|-----------------------|---------------------------------------|---------------------------------------|
|                       | 0.045 to 2 GHz                        | 2 to 18 GHz                           |
| Directivity           | 52                                    | 60                                    |
| Source Match          | 48                                    | 60                                    |
| Load Match            | 52                                    | 60                                    |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^\circ\text{C}$ | $\pm 0.000$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.004$<br>$+0.02/^\circ\text{C}$ | $\pm 0.004$<br>$+0.02/^\circ\text{C}$ |


### Transmission Uncertainty (Specifications) Magnitude

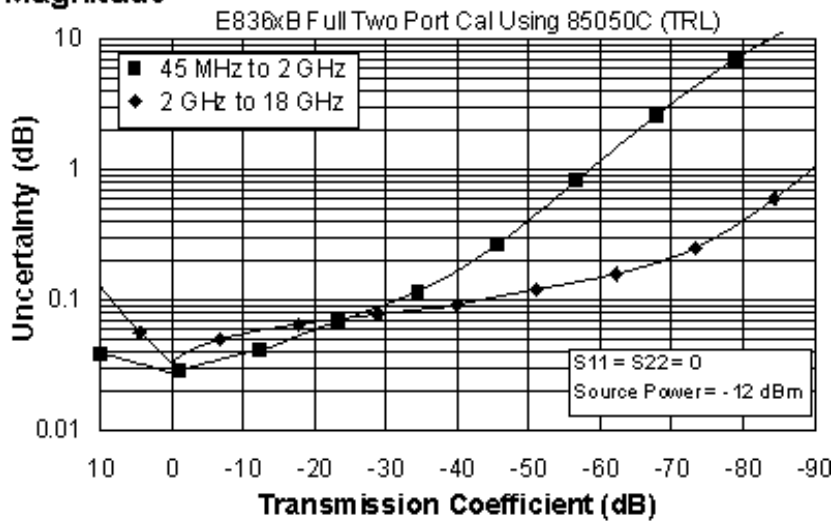


### Phase

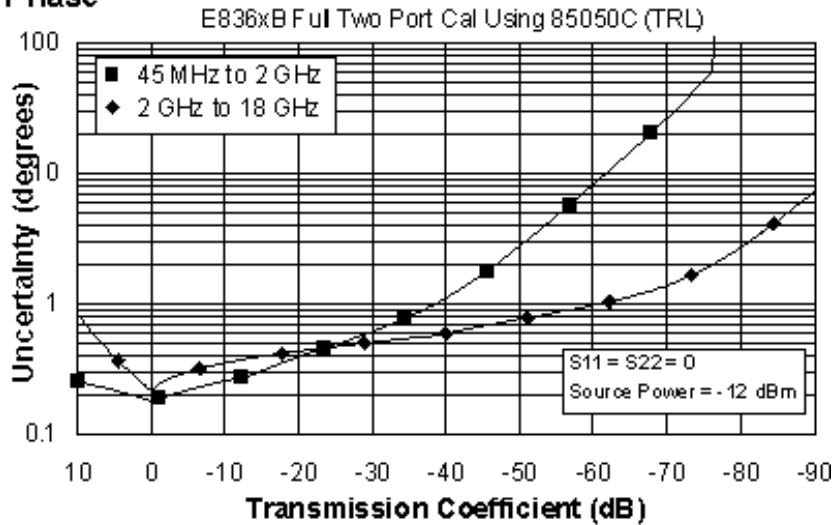

## Reflection Uncertainty (Specifications) Magnitude

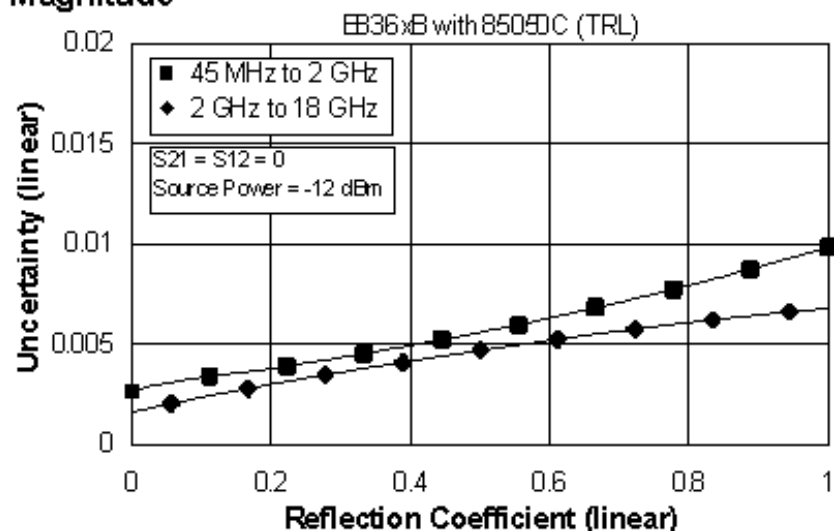

## Phase

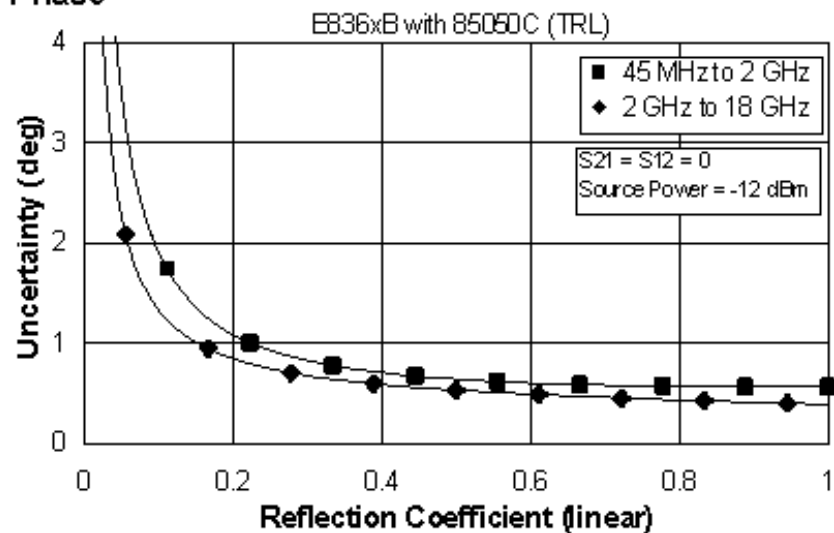

**Table 18. 85050C Calibration Kit**

Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)


Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E836xB analyzers, 85050C (7mm) calibration kit, 85132F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                    |                                       |
|-----------------------|---------------------------------------|---------------------------------------|
|                       | 0.045 to 2 GHz                        | 2 to 18 GHz                           |
| Directivity           | 52                                    | 60                                    |
| Source Match          | 48                                    | 60                                    |
| Load Match            | 52                                    | 60                                    |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^\circ\text{C}$ | $\pm 0.000$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.008$<br>$+0.02/^\circ\text{C}$ | $\pm 0.005$<br>$+0.02/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

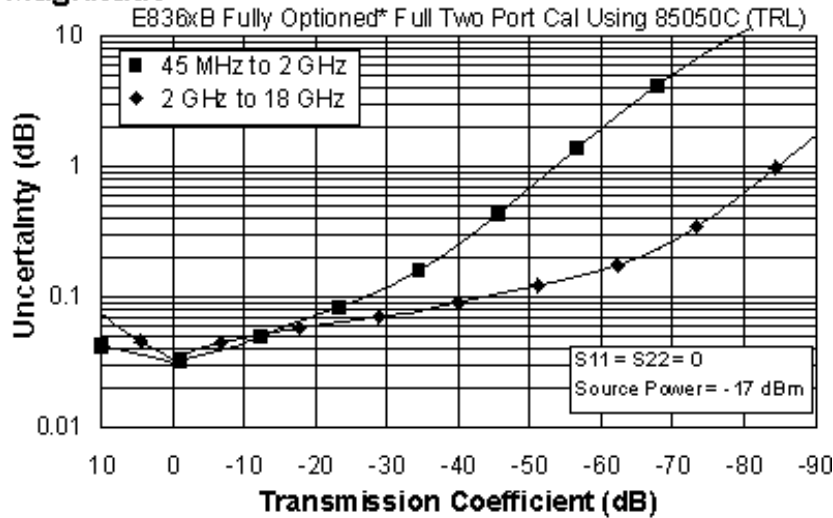

#### Phase

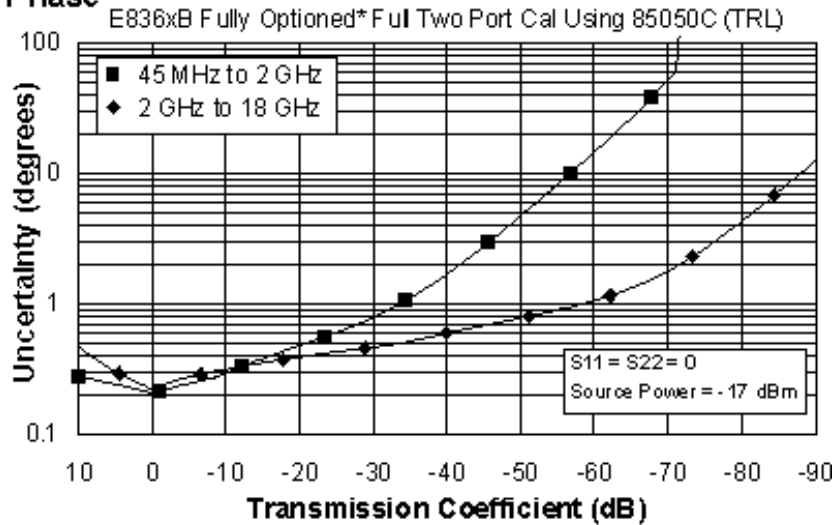





\*Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

**Reflection Uncertainty (Specifications)**

**Magnitude**

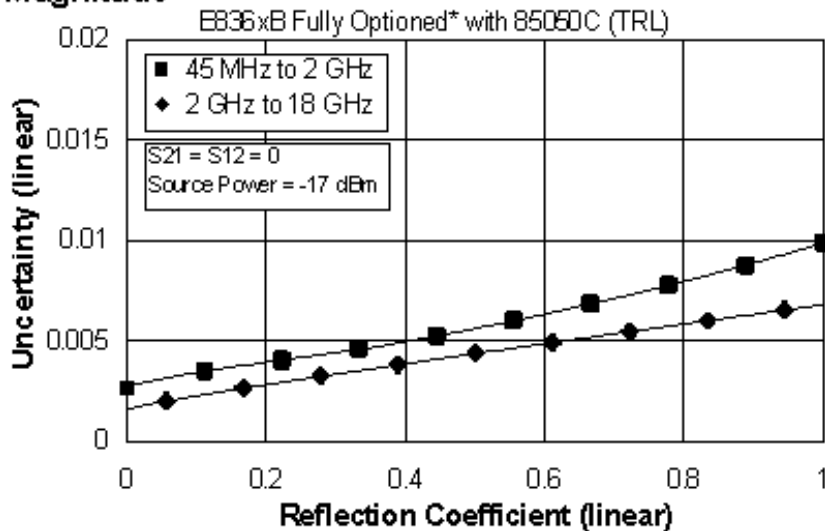

**Phase**

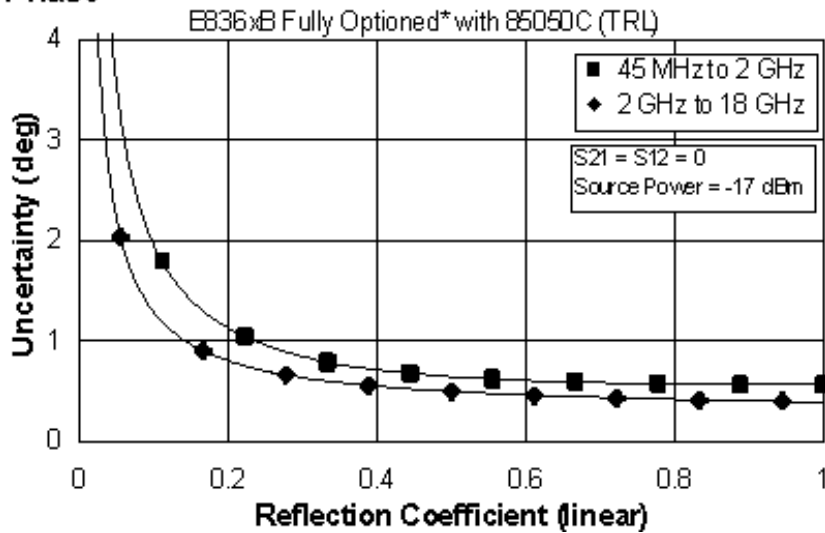

\*Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)


**Table 19. 85050D Calibration Kit**

Standard Configuration and Standard Power Range (E836xB)


Applies to the, E836xB analyzers, 85050D (7mm) calibration kit, 85132F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23 \pm 3$  °C, with < 1 °C deviation from calibration temperature

| Description           | Specification (dB)                    |                                       |
|-----------------------|---------------------------------------|---------------------------------------|
|                       | 0.045 to 2 GHz                        | 2 to 18 GHz                           |
| Directivity           | 40                                    | 40                                    |
| Source Match          | 39                                    | 35                                    |
| Load Match            | 40                                    | 37                                    |
| Reflection Tracking   | $\pm 0.010$<br>$+0.02/^\circ\text{C}$ | $\pm 0.100$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.013$<br>$+0.02/^\circ\text{C}$ | $\pm 0.072$<br>$+0.02/^\circ\text{C}$ |

**Transmission Uncertainty (Specifications)**  
**Magnitude**

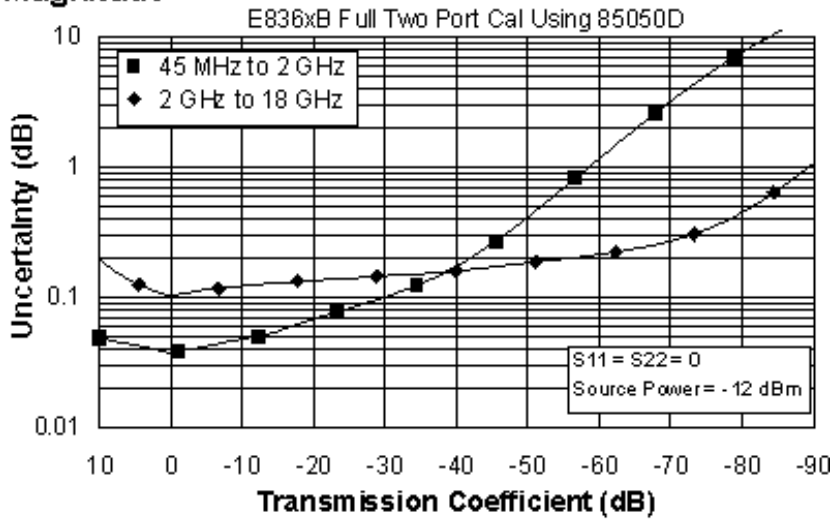


### Phase

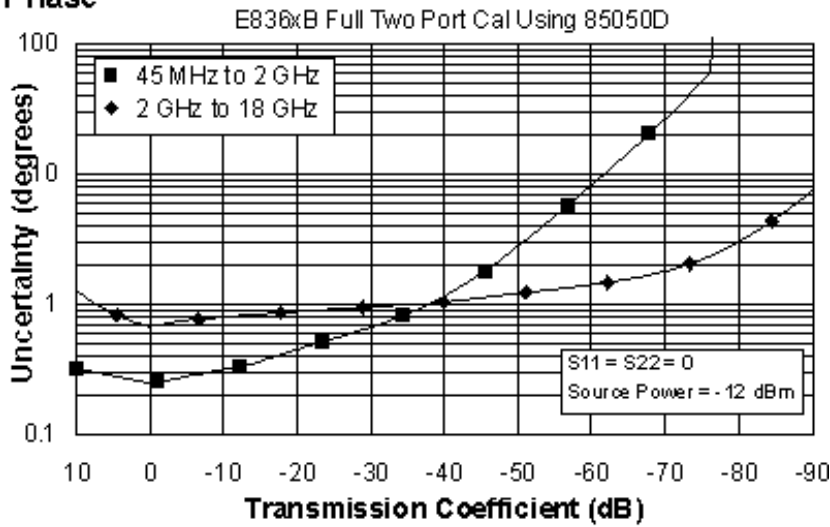


### Reflection Uncertainty (Specifications)

#### Magnitude

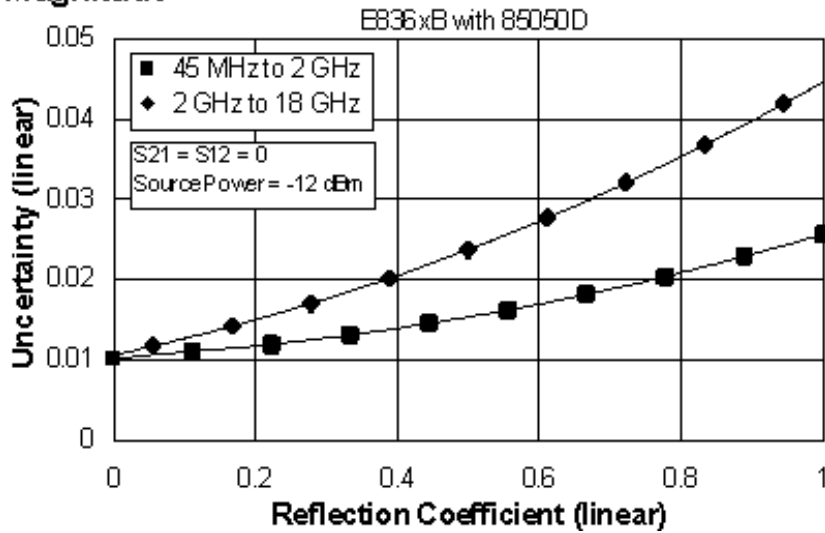

#### Phase

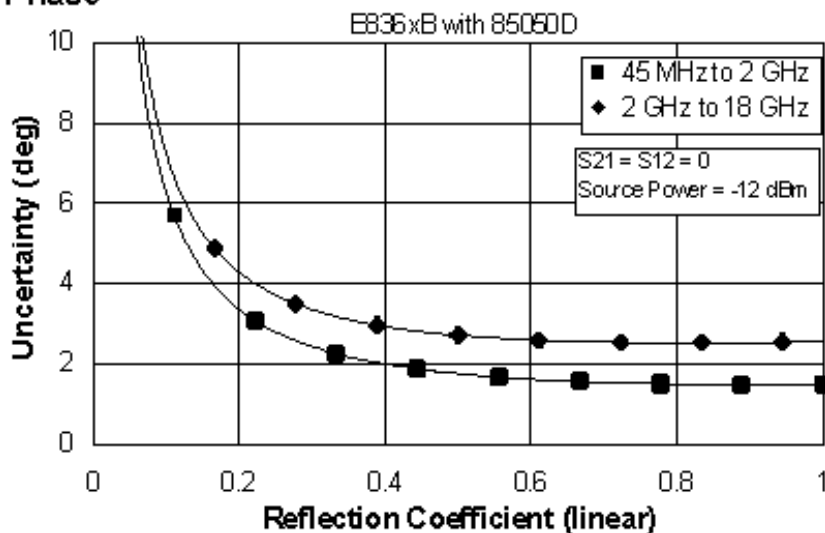

**Table 20.** 85050D Calibration Kit


Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E836xB analyzers, 85050D (7mm) calibration kit, 85132F flexible test port cable set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23 \pm 3$  °C, with  $< 1$  °C deviation from calibration temperature

| Description           | Specification (dB)                    |                                       |
|-----------------------|---------------------------------------|---------------------------------------|
|                       | 0.045 to 2 GHz                        | 2 to 18 GHz                           |
| Directivity           | 40                                    | 40                                    |
| Source Match          | 39                                    | 35                                    |
| Load Match            | 40                                    | 37                                    |
| Reflection Tracking   | $\pm 0.010$<br>$+0.02/^\circ\text{C}$ | $\pm 0.100$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.025$<br>$+0.02/^\circ\text{C}$ | $\pm 0.078$<br>$+0.02/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications) Magnitude

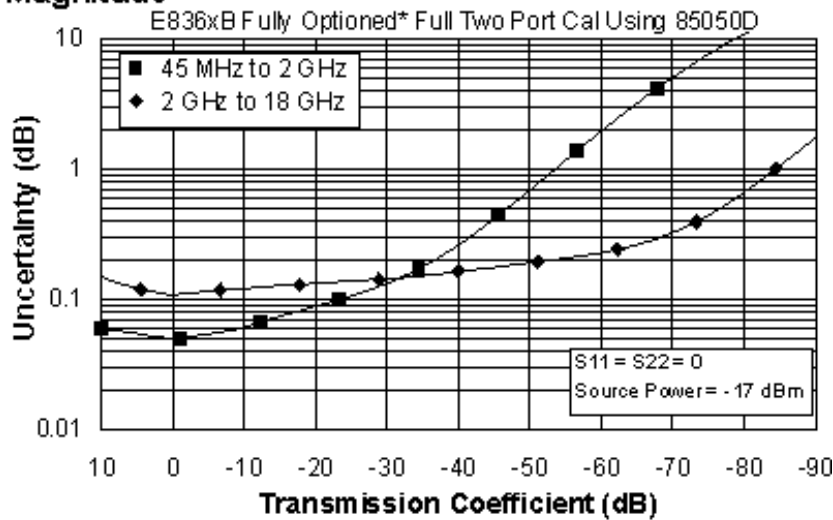


**Phase**

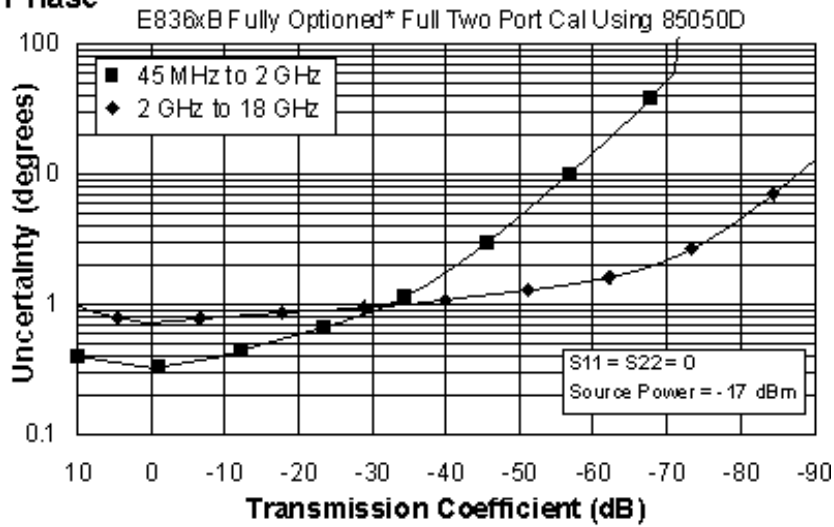


\*Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

**Reflection Uncertainty (Specifications)**

**Magnitude**

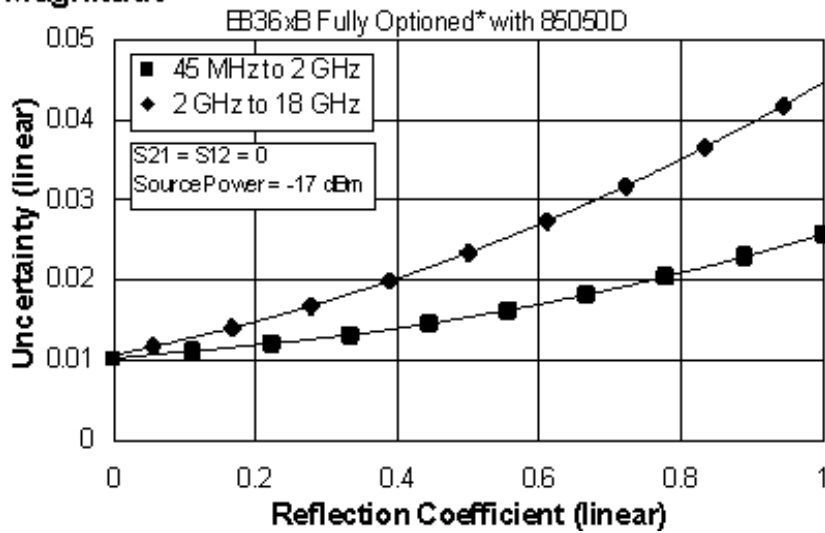

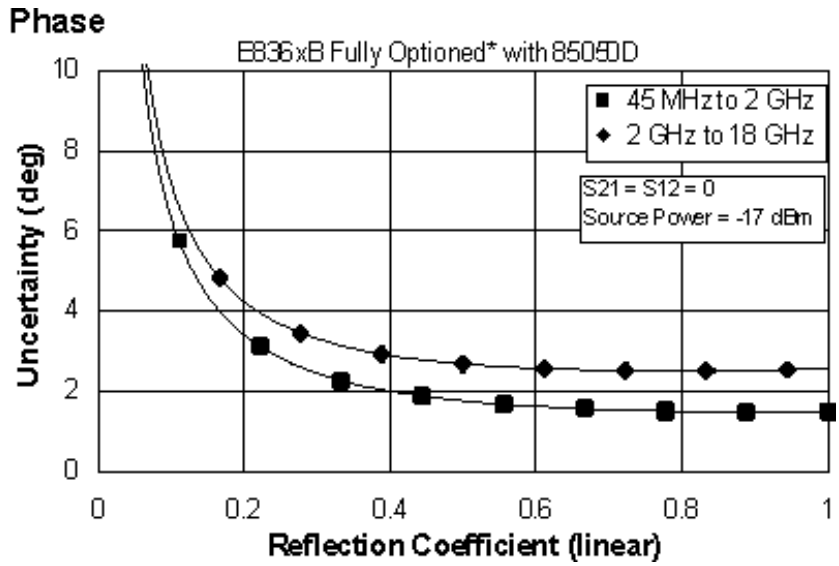

\*Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## E836xB Corrected System Performance with WR-90 Connectors

---

### X11644A Calibration Kit:

#### Standard Configuration and Standard Power Range (E836xB)

#### Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

---

**Table 31.** X11644A Calibration Kit

Standard Configuration and Standard Power Range  
(E836xB)

Applies to the, E836xB analyzers, X11644A (WR-90) calibration kit, 85133F flexible test port cable set with the X281A and X281C launch sets, and a full 2-port calibration. Also applies to the following condition:


Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |
|-----------------------|-----------------------------------------|
|                       | 8.2 to<br>12.4 GHz                      |
| Directivity           | 50                                      |
| Source Match          | 50                                      |
| Load Match            | 50                                      |
| Reflection Tracking   | $\pm 0.000$<br>$+0.02/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.014$<br>$+0.02/^{\circ}\text{C}$ |


### Transmission Uncertainty (Specifications)

---

### Magnitude

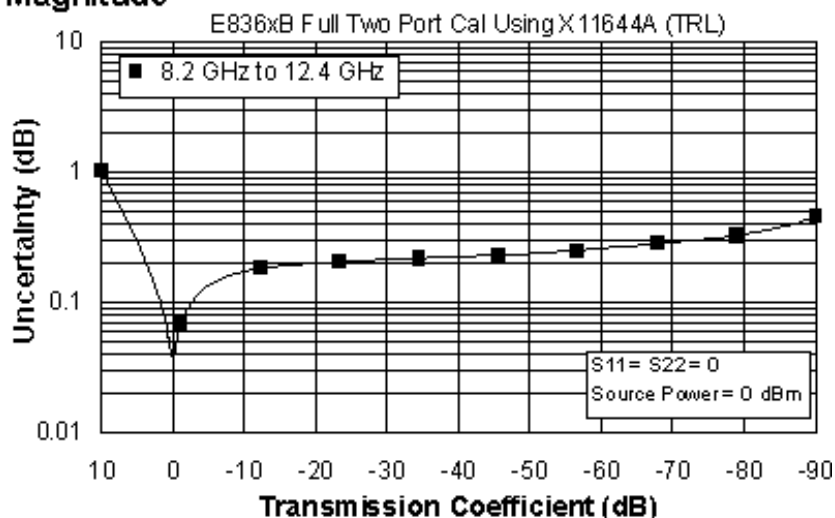


### Phase

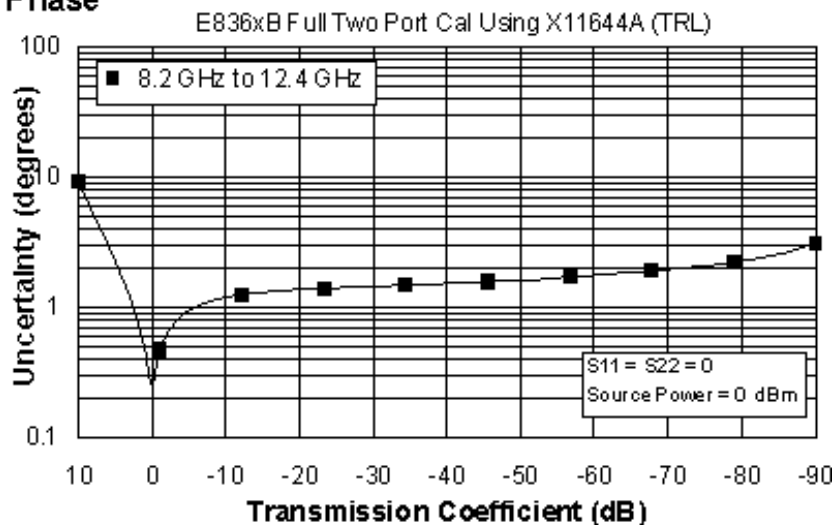


### Reflection Uncertainty (Specifications)

#### Magnitude

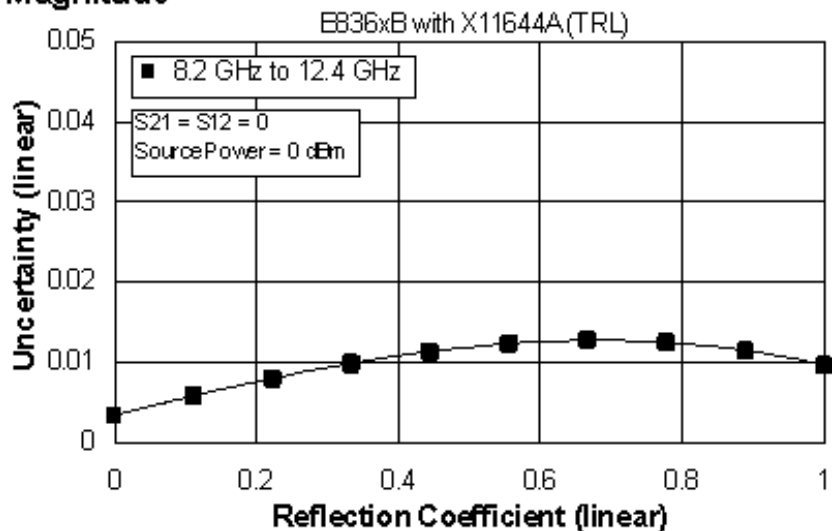



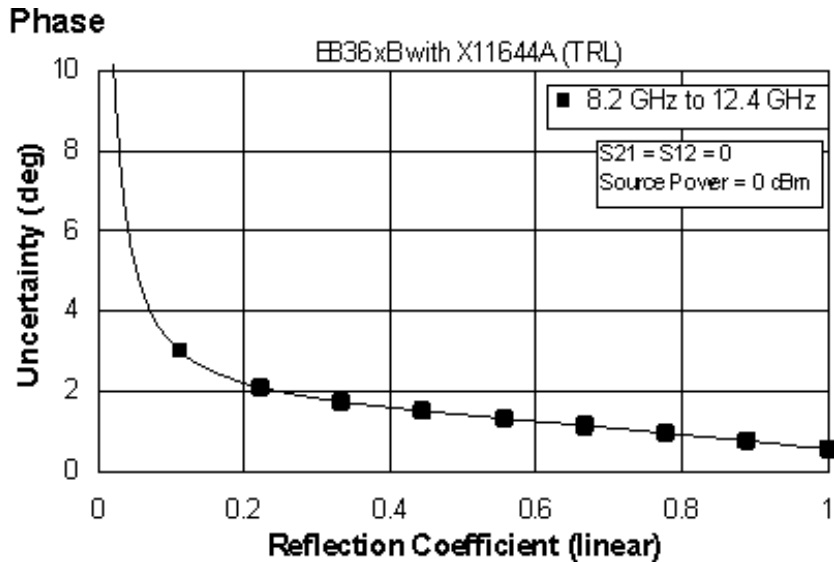

**Table 32. X11644A Calibration Kit**  
Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch


Applies to the, E836xB analyzers, X11644A (WR-90) calibration kit, 85133F flexible test port cable set with the X281A and X281C launch sets, and a full 2-port calibration. Also applies to the following condition:

Environmental temperature 23° ±3 °C, with < 1 °C deviation from calibration temperature


| Description           | Specification (dB)     |
|-----------------------|------------------------|
|                       | <b>8.2 to 12.4 GHz</b> |
| Directivity           | 50                     |
| Source Match          | 50                     |
| Load Match            | 50                     |
| Reflection Tracking   | ±0.000<br>+0.02/°C     |
| Transmission Tracking | ±0.016<br>+0.02/°C     |

### Transmission Uncertainty (Specifications)

## Magnitude

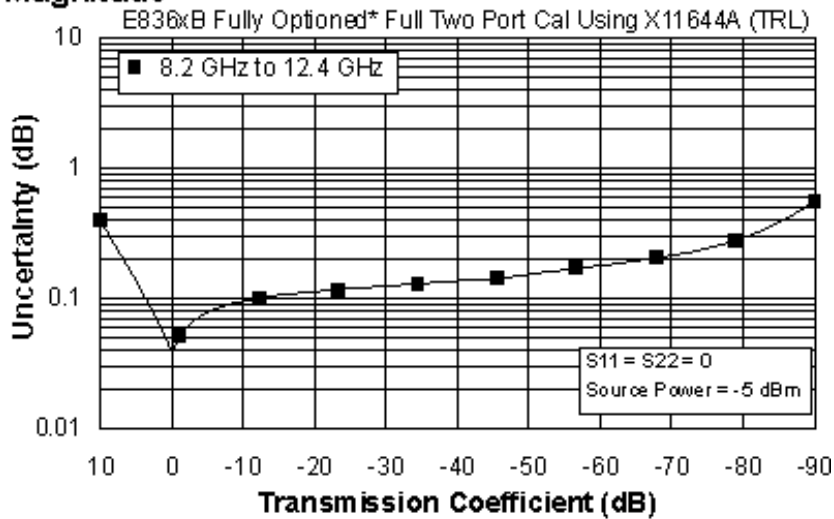


## Phase

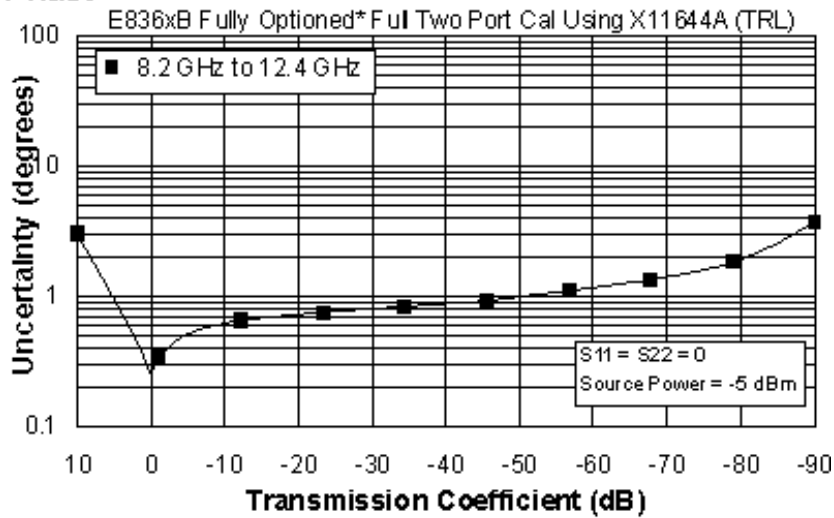


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

## Magnitude

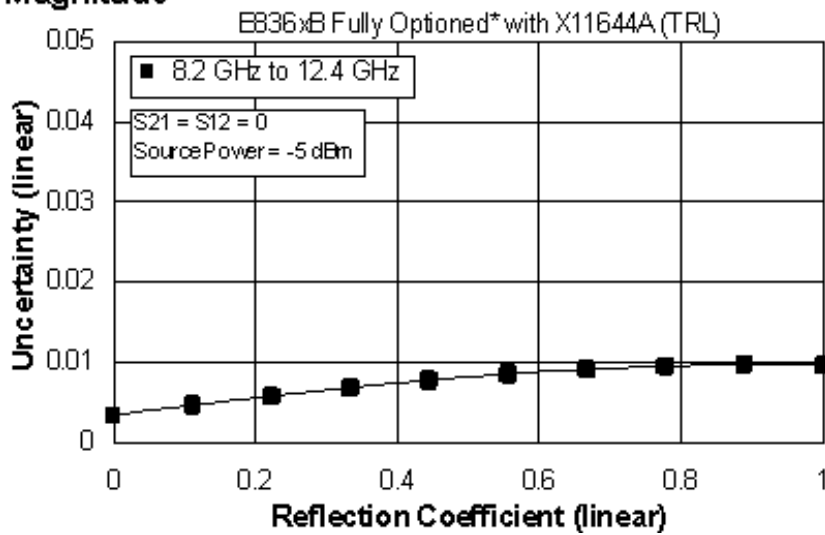

## Phase

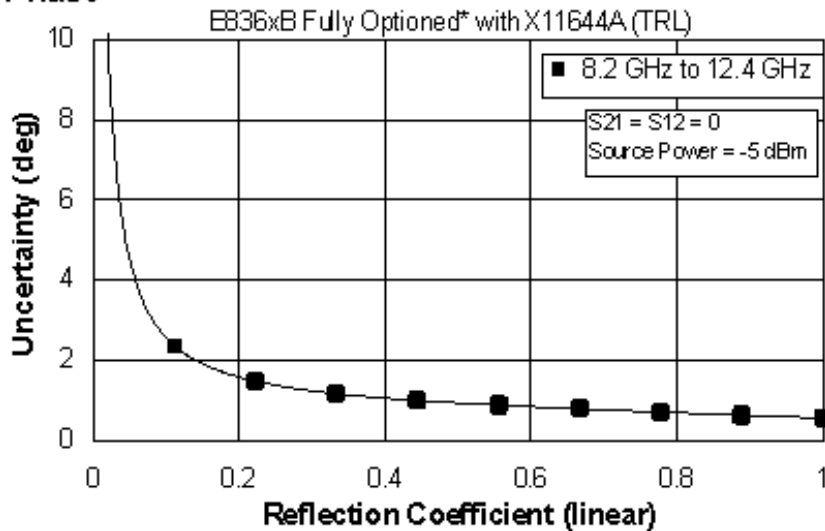

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## E836xB Corrected System Performance with Type-N Connectors

---

### 85054B Calibration Kit:

Standard Configuration and Standard Power Range (E836xB)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

### 85054D Calibration Kit:

Standard Configuration and Standard Power Range (E836xB)

Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

---


**Table 21.** 85054B Calibration Kit  
Standard Configuration and Standard Power Range  
(E836xB)

Applies to the, E836xB analyzers, 85054B (Type-N) calibration kit, 85132F flexible test port cable set with 85130C adapter set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23^{\circ} \pm 3^{\circ}\text{C}$ , with  $< 1^{\circ}\text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|
|                       | 0.045 to<br>2 GHz                       | 2 to<br>18 GHz                          |
| Directivity           | 48                                      | 42                                      |
| Source Match          | 45                                      | 33                                      |
| Load Match            | 48                                      | 41                                      |
| Reflection Tracking   | $\pm 0.001$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.015$<br>$+0.02/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.006$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.079$<br>$+0.02/^{\circ}\text{C}$ |

### Transmission Uncertainty (Specifications)

## Magnitude

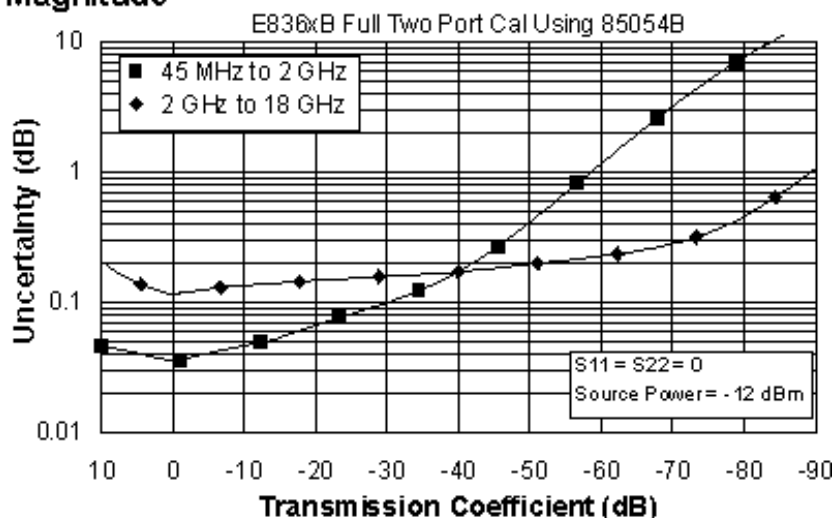



## Phase

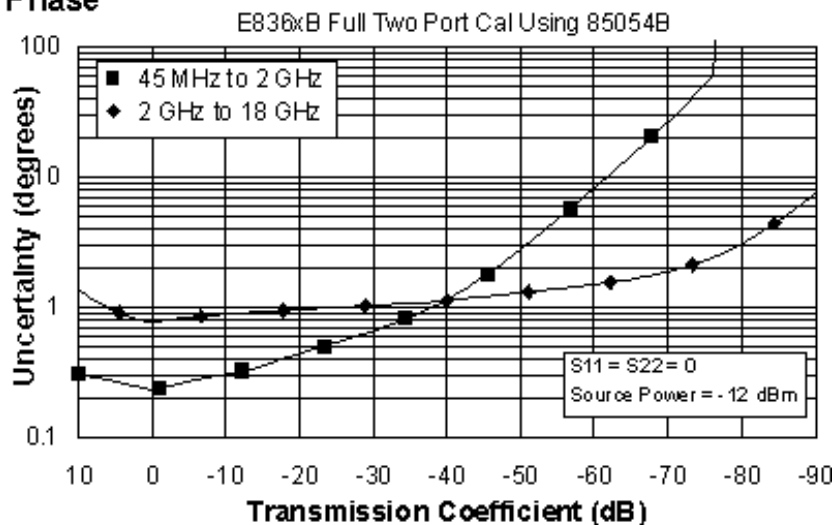

## Reflection Uncertainty (Specifications)

### Magnitude

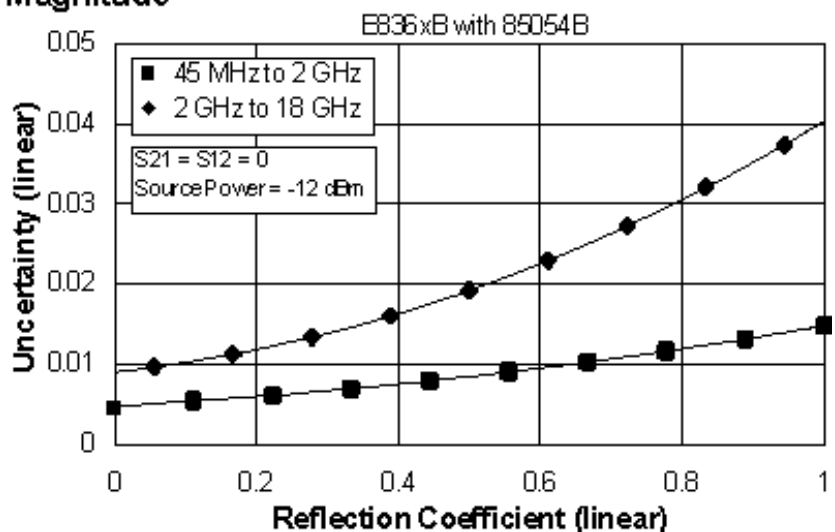

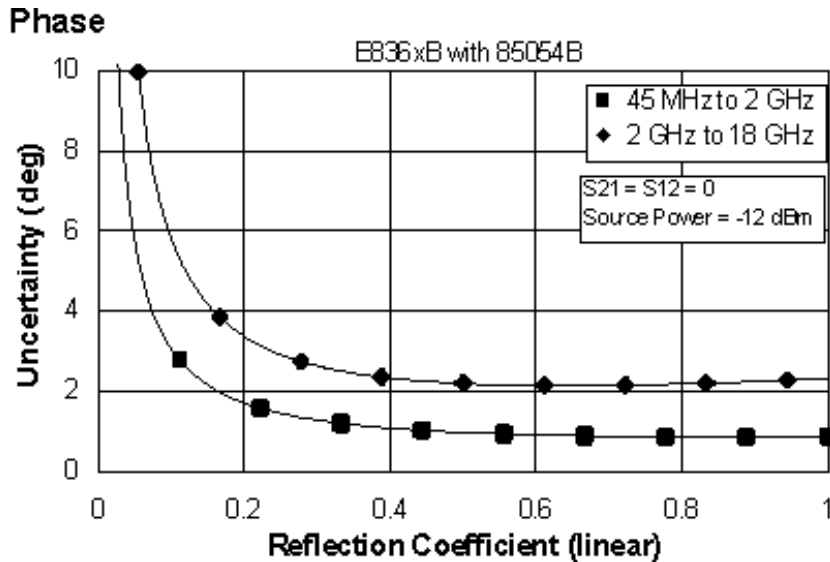


**Table 22. 85054B Calibration Kit**  
 Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)  
 Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E836xB analyzers, 85054B (Type-N) calibration kit, 85132F flexible test port cable set with 85130C adapter set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature


| Description           | Specification (dB)                      |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|
|                       | 0.045 to 2 GHz                          | 2 to 18 GHz                             |
| Directivity           | 48                                      | 42                                      |
| Source Match          | 45                                      | 33                                      |
| Load Match            | 48                                      | 41                                      |
| Reflection Tracking   | $\pm 0.001$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.015$<br>$+0.02/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.011$<br>$+0.02/^{\circ}\text{C}$ | $\pm 0.083$<br>$+0.02/^{\circ}\text{C}$ |

**Transmission Uncertainty (Specifications)**

## Magnitude

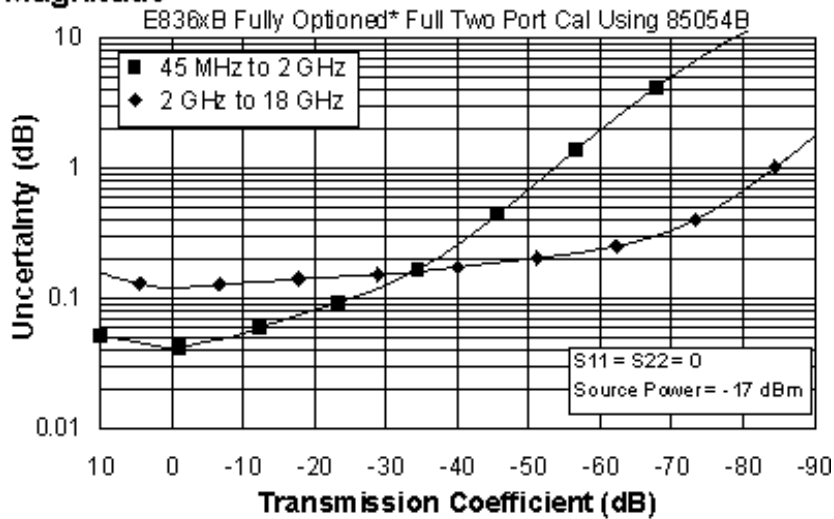


## Phase

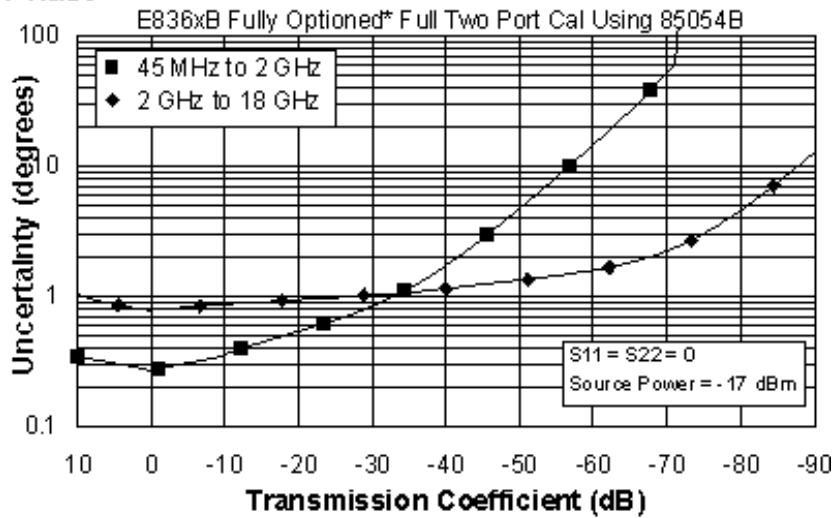


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

## Magnitude

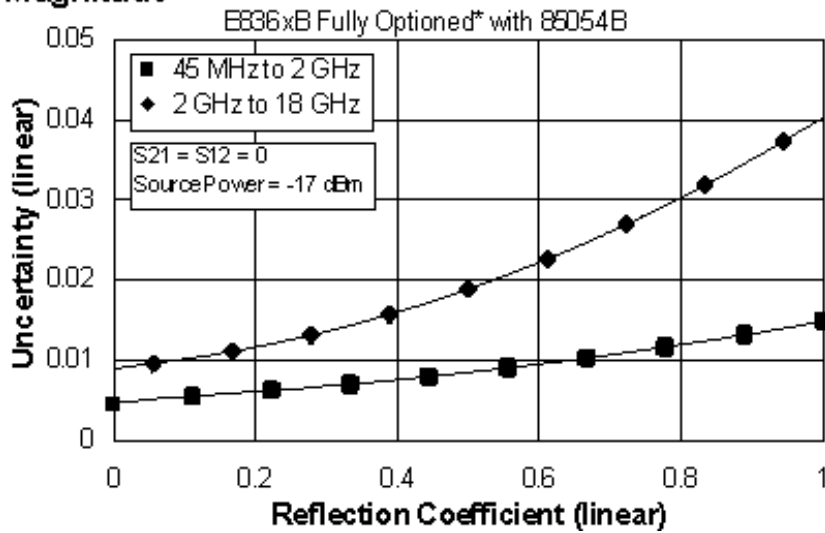

## Phase

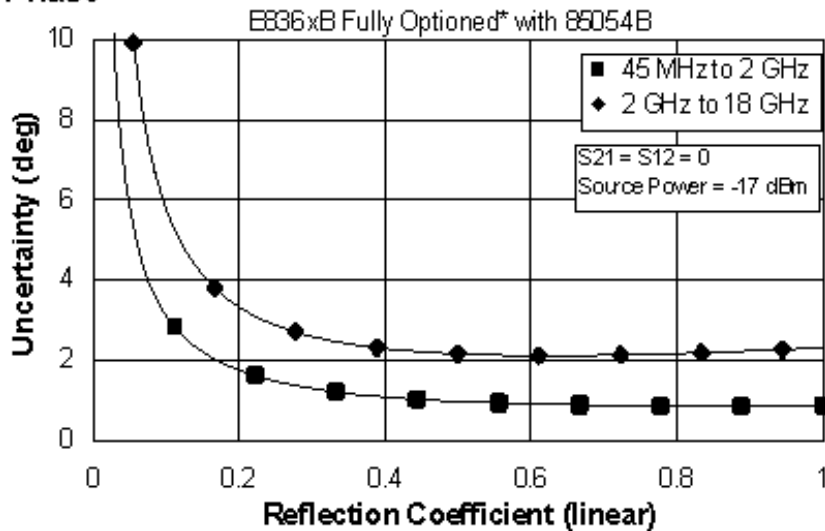

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch (E836xB - Option 014, UNL, 016, 080, and 081)

### Table 23. 85054D Calibration Kit


Standard Configuration and Standard Power Range (E836xB)

Applies to the, E836xB analyzers, 85054D (Type-N) calibration kit, 85132F flexible test port cable set with 85130C adapter set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature




| Description           | Specification (dB)                    |                                       |
|-----------------------|---------------------------------------|---------------------------------------|
|                       | 0.045 to 2 GHz                        | 2 to 18 GHz                           |
| Directivity           | 40                                    | 34                                    |
| Source Match          | 39                                    | 29                                    |
| Load Match            | 40                                    | 34                                    |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^\circ\text{C}$ | $\pm 0.027$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.013$<br>$+0.02/^\circ\text{C}$ | $\pm 0.136$<br>$+0.02/^\circ\text{C}$ |


**Transmission Uncertainty (Specifications)**  
**Magnitude**

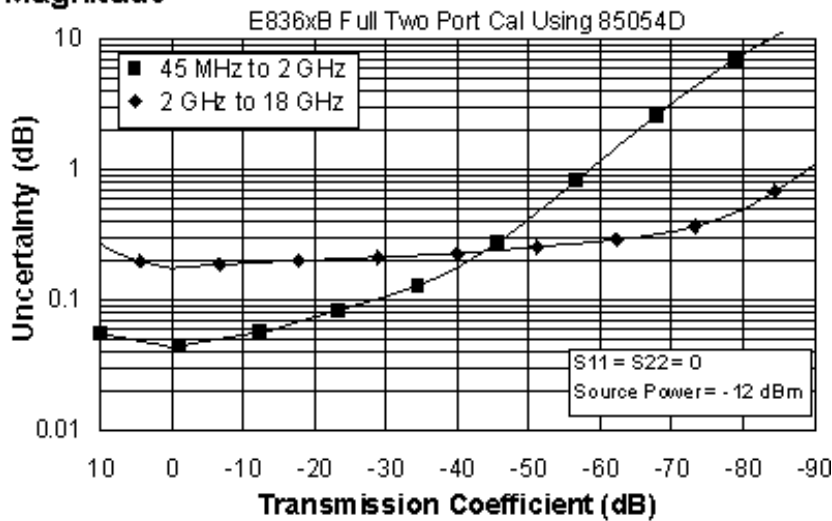


**Phase**

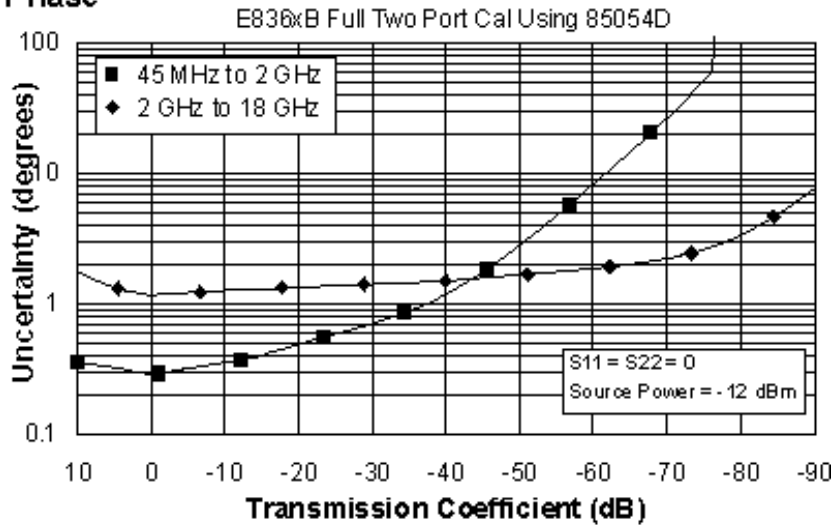

**Reflection Uncertainty (Specifications)**  
**Magnitude**

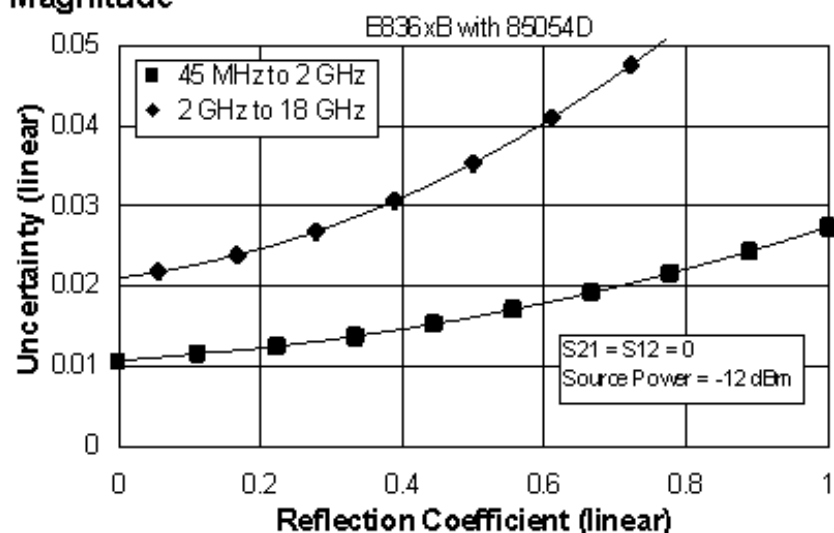

**Phase**

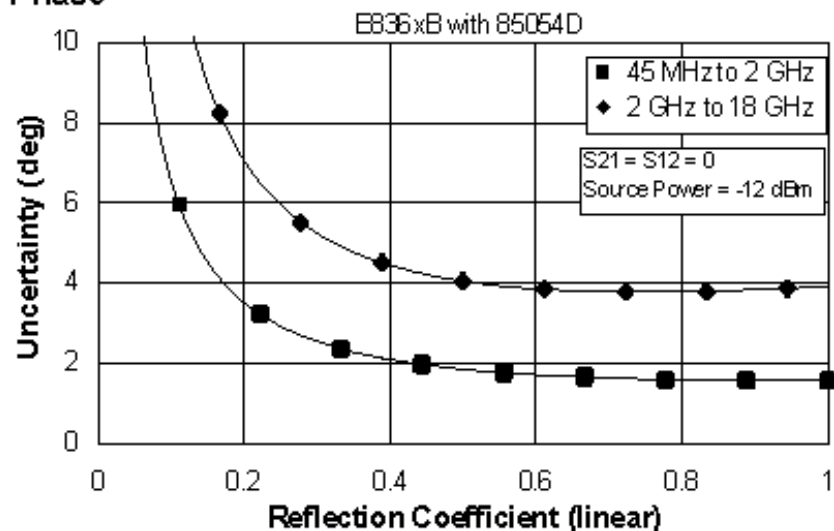

**Table 24. 85054D Calibration Kit**

Fully Optioned (E836xB - Option 014, UNL, 016, 080, and 081)


Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch

Applies to the, E836xB analyzers, 85054D (Type-N) calibration kit, 85132F flexible test port cable set with 85130C adapter set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature 23° ±3 °C, with <1 °C deviation from calibration temperature


| Description           | Specification (dB)                    |                                       |
|-----------------------|---------------------------------------|---------------------------------------|
|                       | 0.045 to<br>2 GHz                     | 2 to<br>18 GHz                        |
| Directivity           | 40                                    | 34                                    |
| Source Match          | 39                                    | 29                                    |
| Load Match            | 40                                    | 34                                    |
| Reflection Tracking   | $\pm 0.003$<br>$+0.02/^\circ\text{C}$ | $\pm 0.027$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.025$<br>$+0.02/^\circ\text{C}$ | $\pm 0.145$<br>$+0.02/^\circ\text{C}$ |

### Transmission Uncertainty (Specifications)

#### Magnitude

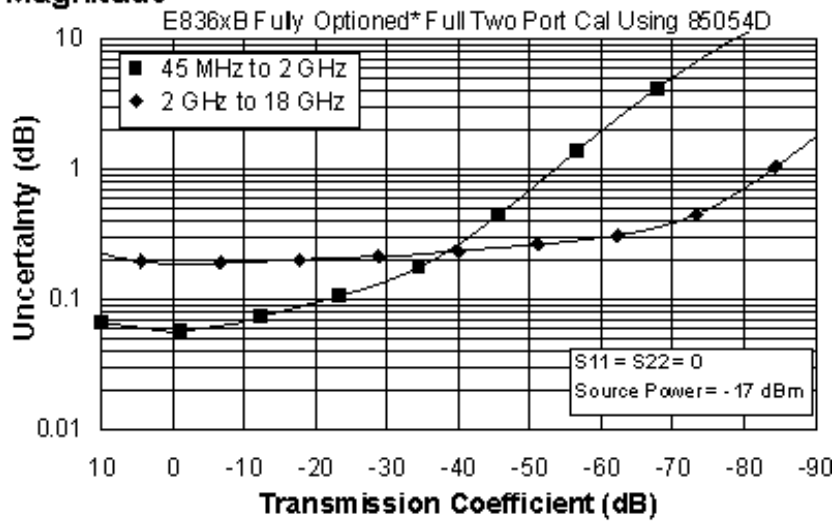


## Phase

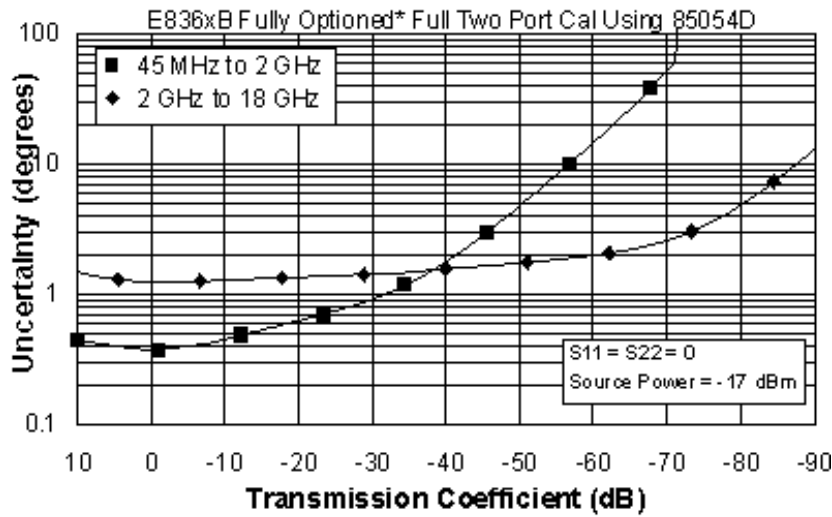


\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
 (E836xB - Option 014, UNL, 016, 080, and 081)

## Reflection Uncertainty (Specifications)

### Magnitude

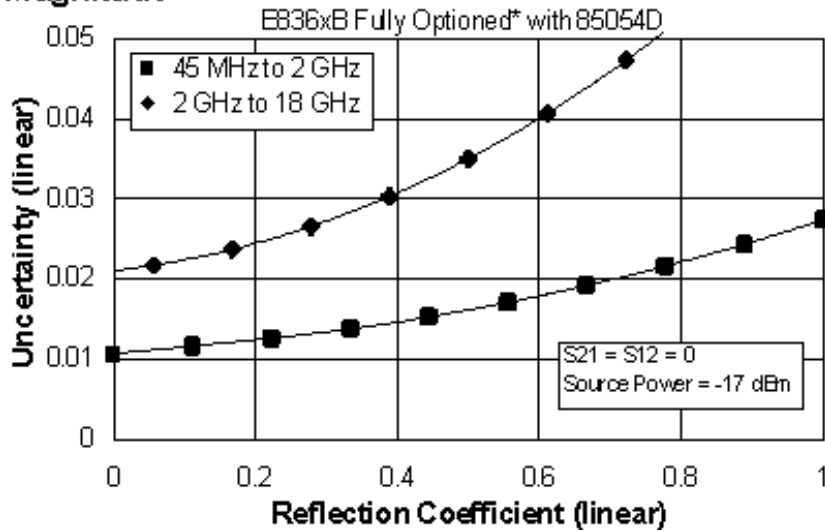

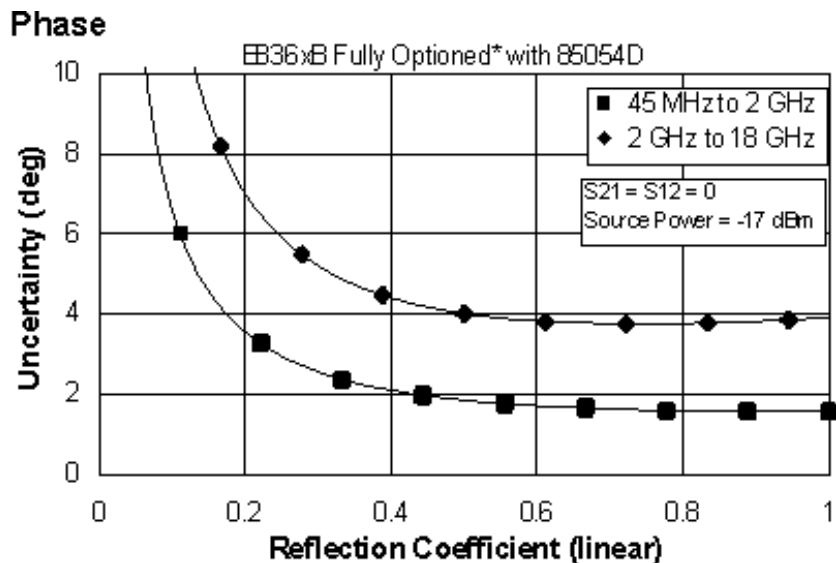

\* Configurable Test Set, Extended Power Range & Bias-Tees, Receiver Attenuators, Frequency Offset Mode, and Reference Channel Transfer Switch  
 (E836xB - Option 014, UNL, 016, 080, and 081)

## N5230A Corrected System Performance with Type-N Connectors

Options 020/025

---

### 85032B Calibration Kit

#### N5230A - Option 020

#### Standard Test Set and Standard Power Range

#### N5230A - Option 025

#### Configurable Test Set and Extended Power Range

---

**Table 13.** 85032B Calibration Kit  
N5230A - Option 020 (Standard Test Set and Standard Power Range)


Applies to the, N5230A Option 020 analyzers, 85032B (Type-N) calibration kit, 85132F flexible test port cable set with 85130C adapter set, and a full 2-port calibration. Also applies to the following condition:  
Environmental temperature  $23 \pm 3$  °C, with  $< 1$  °C deviation from calibration temperature

| Description           | Specification (dB)                    |                                       |                                       |                                       |
|-----------------------|---------------------------------------|---------------------------------------|---------------------------------------|---------------------------------------|
|                       | 0.300 to<br>1 MHz                     | 1 to<br>10 MHz                        | 10 to<br>45 MHz                       | 45 MHz to<br>6 GHz                    |
| Directivity           | 50                                    | 50                                    | 47                                    | 40                                    |
| Source Match          | 42                                    | 42                                    | 37                                    | 31                                    |
| Load Match            | 50                                    | 41                                    | 47                                    | 38                                    |
| Reflection Tracking   | $\pm 0.009$<br>$+0.01/^\circ\text{C}$ | $\pm 0.009$<br>$+0.01/^\circ\text{C}$ | $\pm 0.019$<br>$+0.01/^\circ\text{C}$ | $\pm 0.069$<br>$+0.02/^\circ\text{C}$ |
| Transmission Tracking | $\pm 0.013$<br>$+0.01/^\circ\text{C}$ | $\pm 0.007$<br>$+0.01/^\circ\text{C}$ | $\pm 0.021$<br>$+0.01/^\circ\text{C}$ | $\pm 0.101$<br>$+0.02/^\circ\text{C}$ |


### Transmission Uncertainty (Specifications)

---

## Magnitude

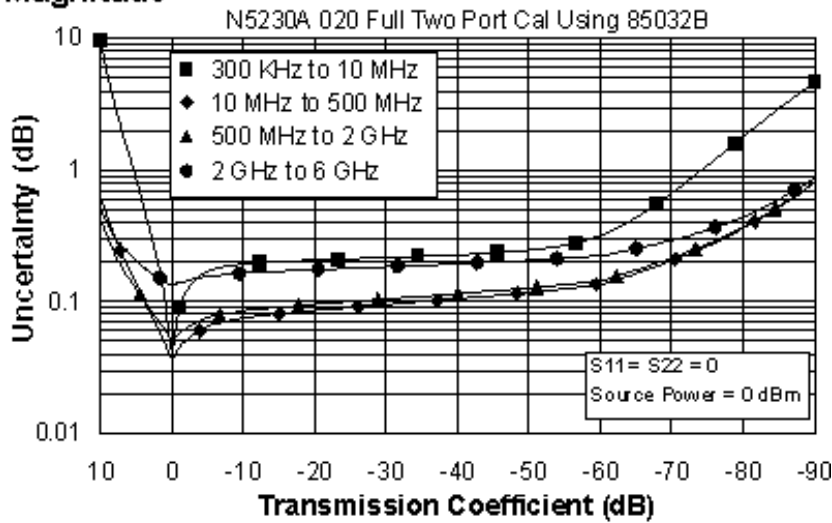


## Phase

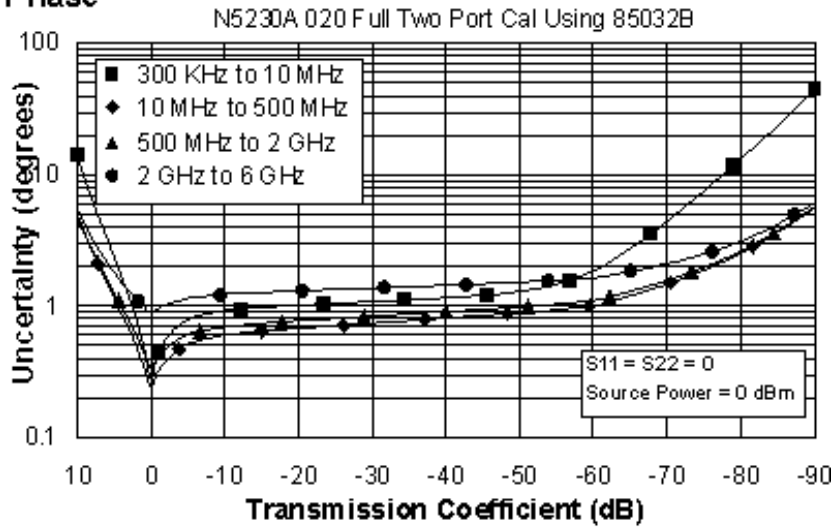


## Reflection Uncertainty (Specifications)

### Magnitude

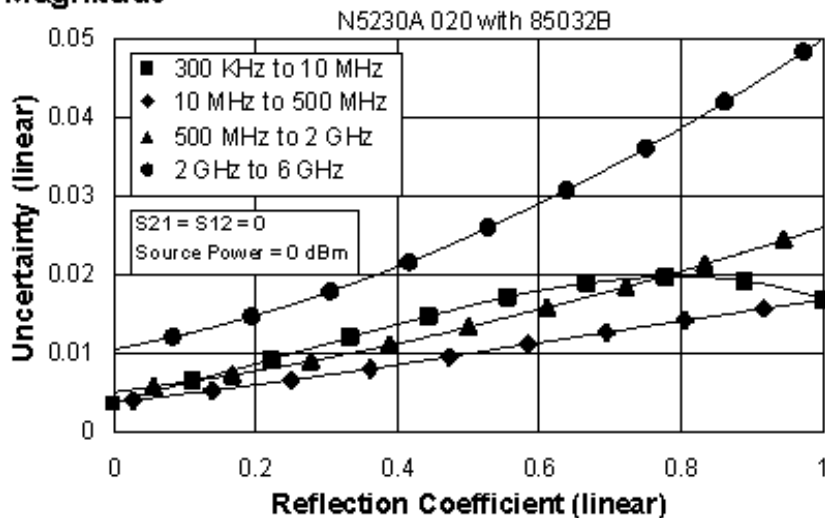

## Phase

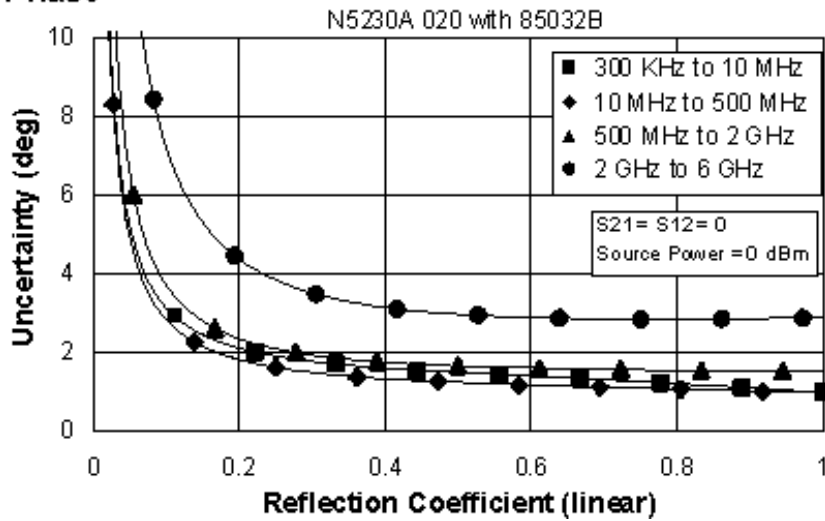

**Table 14.** 85032B Calibration Kit

### N5230A - Option 025 (Configurable Test Set and Extended Power Range)


Applies to the, N5230A Option 025 analyzers, 85032B (Type-N) calibration kit, 85132F flexible test port cable set with 85130C adapter set, and a full 2-port calibration. Also applies to the following condition:  
 Environmental temperature  $23^{\circ} \pm 3^{\circ} \text{C}$ , with  $< 1^{\circ} \text{C}$  deviation from calibration temperature

| Description           | Specification (dB)                      |                                         |                                         |                                         |
|-----------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|-----------------------------------------|
|                       | 0.300 to<br>1 MHz                       | 1 to<br>10 MHz                          | 10 to<br>45 MHz                         | 45 MHz to<br>6 GHz                      |
| Directivity           | 50                                      | 50                                      | 47                                      | 40                                      |
| Source Match          | 42                                      | 42                                      | 37                                      | 31                                      |
| Load Match            | 50                                      | 50                                      | 47                                      | 38                                      |
| Reflection Tracking   | $\pm 0.009$<br>$+0.01/^{\circ}\text{C}$ | $\pm 0.009$<br>$+0.01/^{\circ}\text{C}$ | $\pm 0.019$<br>$+0.01/^{\circ}\text{C}$ | $\pm 0.069$<br>$+0.02/^{\circ}\text{C}$ |
| Transmission Tracking | $\pm 0.013$<br>$+0.01/^{\circ}\text{C}$ | $\pm 0.007$<br>$+0.01/^{\circ}\text{C}$ | $\pm 0.021$<br>$+0.01/^{\circ}\text{C}$ | $\pm 0.101$<br>$+0.02/^{\circ}\text{C}$ |


### Transmission Uncertainty (Specifications)



## Magnitude

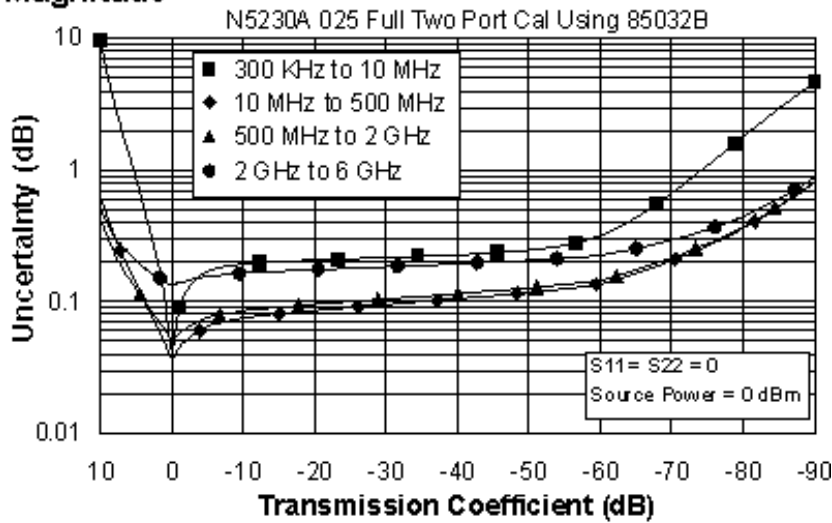


## Phase

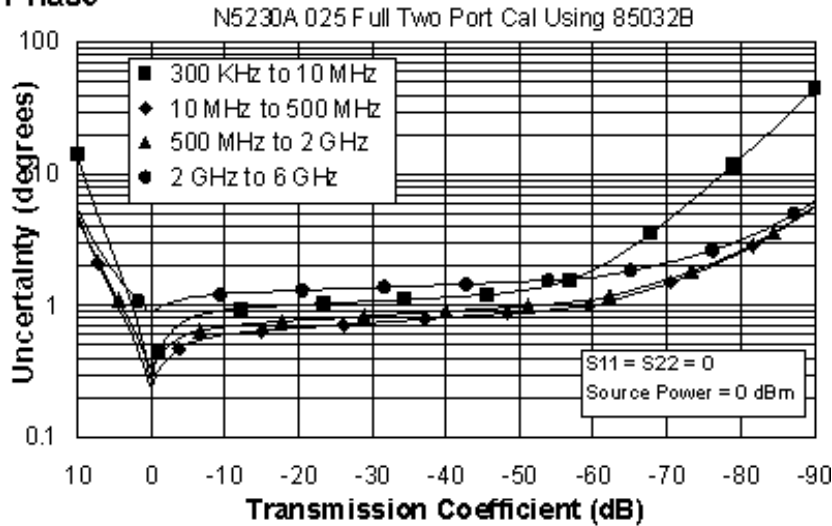


## Reflection Uncertainty (Specifications)

### Magnitude

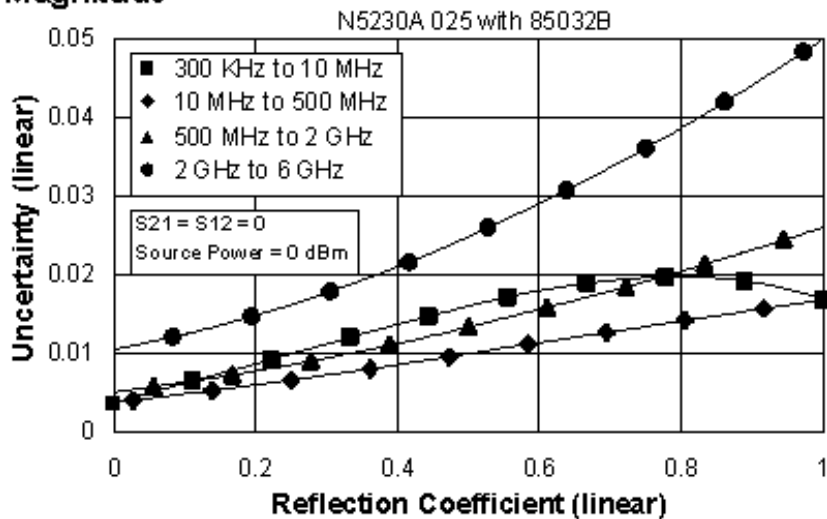

# Phase

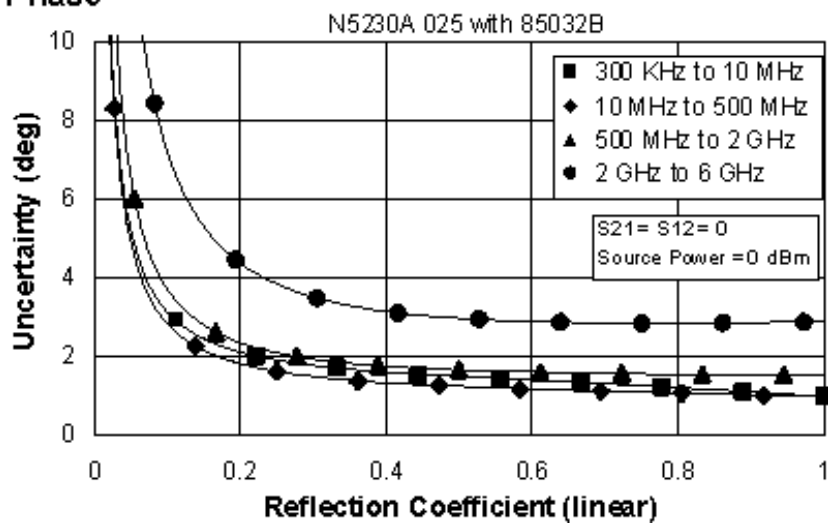

## Equations Used to Generate Uncertainty Curves

---

This topic contains the measurement uncertainty equations used to generate the uncertainty curves in the [Specifications](#) document. It also contains general information about determining system measurement uncertainties.

Learn about the following subjects:

### [Measurement Uncertainty Equations](#)

#### [Forward Reflection Uncertainty](#)

#### [Forward Transmission Uncertainty](#)

#### [Reverse Reflection Uncertainty](#)

#### [Reverse Transmission Uncertainty](#)

### [Sources of Systematic Errors](#)

### [Sources of Random Errors](#)

### [Determining Expected System Performance](#)

### [Determining Cable Stability Terms \(CR1, CR2, CTM1, CTM2, CTP1, CTP2\)](#)

### [Measurement Errors](#)

### [What is Measurement Calibration?](#)

### [Why is Calibration Necessary?](#)

---

## Measurement Uncertainty Equations

Any measurement result is the vector sum of the actual test device response plus all error terms. The precise effect of each error term depends on its magnitude and phase relationship to the actual test device response. When the phase of an error response is not known, phase is assumed to be worst case (-180° to +180°).

View the [abbreviations for residual systematic errors](#) used in the equations.

View the [abbreviations for random errors](#) used in the error models and equations.

### Forward Reflection Uncertainty

#### Equation 1: Forward Reflection Magnitude Uncertainty

$$\Delta S_{11(\text{mag})} = \sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}$$

**Where:**

$$\begin{aligned} \text{Systematic} &= E_{DF} + E_{RF}S_{11} + E_{SF}S_{11}^2 + E_{LF}S_{21}S_{12} + A_M S_{11} \\ \text{Stability} &= \sqrt{C^2 + R^2} \\ C^2 &= C_{RM1}^2(1 + S_{11}^4) + 4C_{TM1}^2 S_{11}^2 + C_{RM2}^2 S_{21}^2 S_{12}^2 \\ R^2 &= (R_{R1}(1 + S_{11}^2) + 2R_{T1}S_{11})^2 + (R_{R2}S_{21}S_{12})^2 \\ \text{Noise}^2 &= (N_T S_{11})^2 + N_F^2 \end{aligned}$$

### Equation 2: Forward Reflection Phase Uncertainty

$$\Delta S_{11(\text{phase})} = \sin^{-1} \left( \frac{\sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}}{S_{11}} \right) + 2C_{TF1}$$

**Where:**

$$\begin{aligned} \text{Systematic} &= E_{DF} + E_{RF}S_{11} + E_{SF}S_{11}^2 + E_{LF}S_{21}S_{12} + \sin(A_P)S_{11} \\ \text{Stability} &= \sqrt{C^2 + R^2} \\ C^2 &= C_{RM1}^2(1 + S_{11}^4) + 4C_{TM1}^2 S_{11}^2 + C_{RM2}^2 S_{21}^2 S_{12}^2 \\ R^2 &= (R_{R1}(1 + S_{11}^2) + 2R_{T1}S_{11})^2 + (R_{R2}S_{21}S_{12})^2 \\ \text{Noise}^2 &= (N_T S_{11})^2 + N_F^2 \end{aligned}$$

Forward Transmission Uncertainty

### Equation 3: Forward Transmission Magnitude Uncertainty

$$\Delta S_{21(\text{mag})} = \sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}$$

**Where:**

$$\begin{aligned} \text{Systematic} &= E_{XF} + S_{21}(E_{TF} + E_{SF}S_{11} + E_{LF}S_{22} + E_{SF}E_{LF}S_{21}S_{12} + A_M) \\ \text{Stability} &= \sqrt{C^2 + R^2} \\ C^2 &= S_{21}^2(C_{TM1}^2 + C_{TM2}^2 + (C_{R1}S_{11})^2 + (C_{R2}S_{22})^2) \\ R^2 &= S_{21}^2((R_{T1} + R_{R1}S_{11})^2 + (R_{T2} + R_{R2}S_{22})^2) \\ \text{Noise}^2 &= (N_T S_{21})^2 + N_F^2 \end{aligned}$$

### Equation 4: Forward Transmission Phase Uncertainty

$$\Delta S_{21(\text{phase})} = \sin^{-1} \left( \frac{\sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}}{S_{21}} \right) + C_{TF1} + C_{TF2}$$

**Where:**

$$\begin{aligned} \text{Systematic} &= E_{XF} + S_{21}(E_{TF} + E_{SF}S_{11} + E_{LF}S_{22} + E_{SF}E_{LF}S_{21}S_{12} + \sin(A_P)) \\ \text{Stability} &= \sqrt{C^2 + R^2} \\ C^2 &= S_{21}^2(C_{TM1}^2 + C_{TM2}^2 + (C_{R1}S_{11})^2 + (C_{R2}S_{22})^2) \\ R^2 &= S_{21}^2((R_{T1} + R_{R1}S_{11})^2 + (R_{T2} + R_{R2}S_{22})^2) \\ \text{Noise}^2 &= (N_T S_{21})^2 + N_F^2 \end{aligned}$$

### Reverse Reflection Uncertainty

### Equation 5: Reverse Reflection Magnitude Uncertainty

$$\Delta S_{22(\text{mag})} = \sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}$$

**Where:**

$$\text{Systematic} = E_{DR} + E_{RR}S_{22} + E_{SR}S_{22}^2 + E_{LR}S_{21}S_{12} + A_M S_{22}$$

$$\text{Stability} = \sqrt{C^2 + R^2}$$

$$C^2 = C_{RM2}^2(1 + S_{22}^A) + 4C_{TM2}^2S_{22}^2 + C_{RM1}^2S_{21}^2S_{12}^2$$

$$R^2 = (R_{R2}(1 + S_{22}^2) + 2R_{T2}S_{22})^2 + (R_{R1}S_{21}S_{12})^2$$

$$\text{Noise}^2 = (N_T S_{22})^2 + N_F^2$$

### Equation 6: Reverse Reflection Phase Uncertainty

$$\Delta S_{22(\text{phase})} = \sin^{-1}\left(\frac{\sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}}{S_{22}}\right) + 2C_{TF2}$$

**Where:**

$$\text{Systematic} = \frac{E_{DR} + E_{RR}S_{22} + E_{SR}S_{22}^2 + E_{LR}S_{21}S_{12} + \sin(A_P)S_{22}}{S_{22}}$$

$$\text{Stability} = \sqrt{C^2 + R^2}$$

$$C^2 = C_{RM2}^2(1 + S_{22}^A) + 4C_{TM2}^2S_{22}^2 + C_{RM1}^2S_{21}^2S_{12}^2$$

$$R^2 = (R_{R2}(1 + S_{22}^2) + 2R_{T2}S_{22})^2 + (R_{R1}S_{21}S_{12})^2$$

$$\text{Noise}^2 = (N_T S_{22})^2 + N_F^2$$

### Reverse Transmission Uncertainty

#### Equation 7: Reverse Transmission Magnitude Uncertainty

$$\Delta S_{12(\text{mag})} = \sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}$$

**Where:**

$$\text{Systematic} = \frac{E_{XR} + S_{12}(E_{TR} + E_{SR}S_{22} + E_{LR}S_{11} + E_{SR}E_{LR}S_{21}S_{12} + A_M)}{S_{12}}$$

$$\text{Stability} = \sqrt{C^2 + R^2}$$

$$C^2 = S_{12}^2(C_{TM1}^2 + C_{TM2}^2 + (C_{R1}S_{11})^2 + (C_{R2}S_{22})^2)$$

$$R^2 = S_{12}^2((R_{T1} + R_{R1}S_{11})^2 + (R_{T2} + R_{R2}S_{22})^2)$$

$$\text{Noise}^2 = (N_T S_{12})^2 + N_F^2$$

#### Equation 8: Reverse Transmission Phase Uncertainty

$$\Delta S_{12(\text{phase})} = \sin^{-1}\left(\frac{\sqrt{(\text{Systematic} + \text{Stability})^2 + \text{Noise}^2}}{S_{12}}\right) + C_{TF1} + C_{TF2}$$

**Where:**

$$\text{Systematic} = E_{XR} + S_{12}(E_{TR} + E_{SR}S_{22} + E_{LR}S_{11} + E_{SR}E_{LR}S_{21}S_{12} + \sin(A_P))$$

$$\text{Stability} = \sqrt{C^2 + R^2}$$

$$C^2 = S_{12}^2(C_{TM1}^2 + C_{TM2}^2 + (C_{R1}S_{11})^2 + (C_{R2}S_{22})^2)$$

$$R^2 = S_{12}^2((R_{T1} + R_{R1}S_{11})^2 + (R_{T2} + R_{R2}S_{22})^2)$$

$$\text{Noise}^2 = (N_T S_{12})^2 + N_F^2$$

## Sources of Systematic Errors

The residual (after measurement calibration) **systematic errors** result from imperfections in the calibration standards.

For **reflection measurements**, the associated residual errors are:

- residual directivity
- residual load match
- residual source match
- residual reflection tracking

For **transmission measurements**, the additional residual errors are:

- residual crosstalk
- residual load match
- residual source match
- residual transmission tracking

The listing below shows the **abbreviations** used for residual systematic errors that are in the uncertainty equations.

- **EDF** = forward residual directivity
- **ESR** = reverse residual source match
- **ESF** = forward residual source match
- **ERR** = reverse residual reflection tracking
- **ERF** = forward residual reflection tracking
- **EXR** = reverse crosstalk
- **EXF** = forward crosstalk
- **ELR** = reverse load match
- **ELF** = forward load match
- **ETR** = reverse transmission tracking
- **ETF** = forward transmission tracking
- **AM** = magnitude dynamic accuracy
- **EDR** = reverse residual directivity
- **AP** = phase dynamic accuracy

All measurements are affected by **dynamic accuracy**. Dynamic accuracy includes: errors during internal self-calibration routines, gain compression in the microwave frequency converter (sampler) at high signal levels, errors generated in the synchronous detectors, localized non-linearities in the IF filter system, and from LO leakage into the IF signal paths.

## Sources of Random Errors

The **random error** sources are

- noise
- connector repeatability

- interconnecting cable stability

There are two types of noise in any measurement system:

1. low level noise (noise floor)
2. high level noise (trace noise)

**Low level noise** is the broadband noise floor of the receiver which can be reduced through averaging or by changing the IF bandwidth.

**High level noise** or trace noise is due to the noise floor of the receiver, and the phase noise of the LO source inside the test set. It is worsened by reducing the IF bandwidth. Using a high stability 10 MHz time base can reduce high level noise.

A high stability time base is standard with PNA models E8356/7/8A and E8362/3/4A. It is available as Option 1E5 with PNA models E8801/2/3A and N3381/2/3A. Option 1E5 replaces a 10 ppm time base with a 1 ppm time base.

**Connector repeatability** is the random variation encountered when connecting a pair of RF connectors. Variations in both reflection and transmission can be observed.

**Cable stability** is dependent on the cable used and the amount of cable movement between calibration and measurement.

The listing below shows the **abbreviations** used for random errors in the error models and uncertainty equations.

- |                                                               |                                                               |
|---------------------------------------------------------------|---------------------------------------------------------------|
| ○ <b>NF</b> = noise floor                                     | ○ <b>CTM2</b> = port 2 cable magnitude transmission stability |
| ○ <b>NT</b> = trace noise                                     | ○ <b>CTP2</b> = port 2 cable phase transmission stability     |
| ○ <b>CR1</b> = port 1 cable reflection stability              | ○ <b>RR1</b> = port 1 connector reflection repeatability      |
| ○ <b>CTM1</b> = port 1 cable magnitude transmission stability | ○ <b>RT1</b> = port 1 connector transmission repeatability    |
| ○ <b>CTP1</b> = port 1 cable phase transmission stability     | ○ <b>RR2</b> = port 2 connector reflection repeatability      |
| ○ <b>CR2</b> = port 2 cable reflection stability              | ○ <b>RT2</b> = port 2 connector transmission repeatability    |

## Determining Expected System Performance

Improper connection techniques and contact surfaces can degrade measurement accuracy.

Proper connection techniques include using a torque wrench with proper torque limits, ensuring that the connector pin depths meet specifications, ensuring that the center conductor of sliding loads is properly set, and observing proper handling procedures for beadless airlines.

Contact surface errors are caused by improper cleaning procedures, scratches, worn plating, and rough seating.

View more information on [connector care](#)

If proper connection techniques and connector care is observed, the following table provides an indication of connector repeatability.

| Connector Repeatability ( $R_{R1}$ , $R_{R2}$ , $R_{T1}$ , and $R_{T2}$ ) |               |  |                 |               |
|---------------------------------------------------------------------------|---------------|--|-----------------|---------------|
| Connector Type                                                            |               |  | Connector Type  |               |
| Frequency Range                                                           | Repeatability |  | Frequency Range | Repeatability |
| 2.4-mm                                                                    |               |  | 3.5-mm          |               |
| 0 to 2 GHz                                                                | 0.0002        |  | 0 to 2 GHz      | 0.0001        |
| 2 to 20 GHz                                                               | 0.0004        |  | 2 to 8 GHz      | 0.0003        |
| 20 to 36 GHz                                                              | 0.0006        |  | 8 to 20 GHz     | 0.0006        |
| 36 to 40 GHz                                                              | 0.0008        |  | 20 to 26.5 GHz  | 0.0010        |
| 7-mm                                                                      |               |  | Type-N          |               |
| 0 to 2 GHz                                                                | 0.0001        |  | 0 to 2 GHz      | 0.0006        |
| 2 to 8 GHz                                                                | 0.0003        |  | 2 to 8 GHz      | 0.0006        |
| 8 to 18 GHz                                                               | 0.0006        |  | 8 to 18 GHz     | 0.0010        |
| Type-F                                                                    |               |  | Waveguide       |               |
| 0 to 3 GHz                                                                | 0.0006        |  | 0 to 40 GHz     | 0.0002        |

### Determining Cable Stability Terms ( $CR_1$ , $CR_2$ , $CTM_1$ , $CTM_2$ , $CTP_1$ , $CTP_2$ )


Cable stability is dependent on the cable used and the amount of cable movement between calibration and measurement. Values for **cable reflection stability** are determined by connecting a fixed load to the free end of the cable and measuring the change in reflection coefficient after flexing the cable through the normal range of cable movement for a particular setup. **Cable transmission stability** is determined by connecting a short to the free end of the cable and measuring the change in reflection coefficient due to changes in cable position.

Graphics 1-3 demonstrate concepts useful in determining cable stability. In each case, a cable (part number 8120-4779) was connected to port 1, with a fixed load connected to the free end. A reference trace is obtained by measuring  $S_{11}$  with the free end held close to port 2 and storing the results in memory. Two additional  $S_{11}$  measurements are made; one with the cable flexed out to its straight position and the other with the cable positioned back to the same location as reference trace. As shown in Graphic 1, the flexed position demonstrates the effect of moving the cable after calibration. The repeatability trace demonstrates the stability of the cable when moved to its original position.

#### Graphic 1




### Cable Stability with Fixed Load Connected

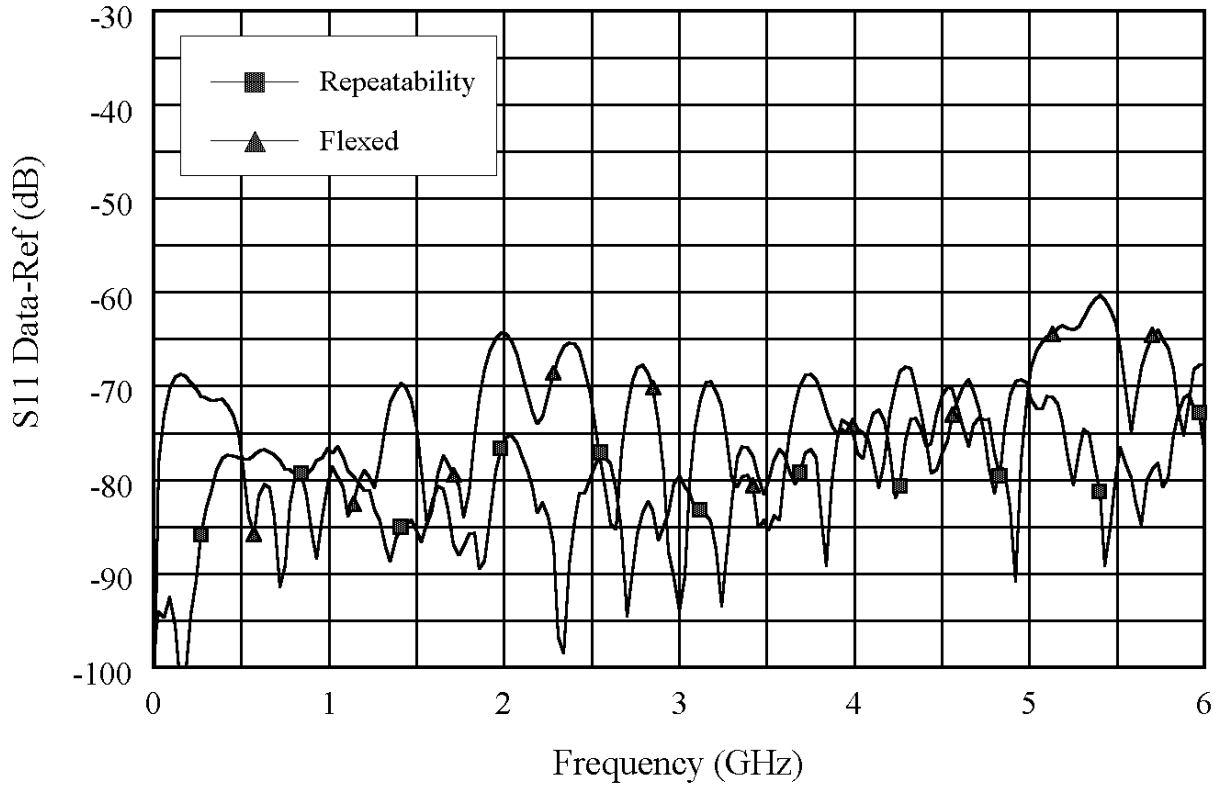

Graphic 1 demonstrates the concepts useful in determining cable reflection stability. A fixed load is connected to the free end. The DATA-MEM feature provides an indication of the cable reflection stability. A 60-dB peak on the chart yields a reflection stability estimated as  $10^{(-60/20)}$  or 0.001.

### Graphic 2


### Cable Stability with Short Connected

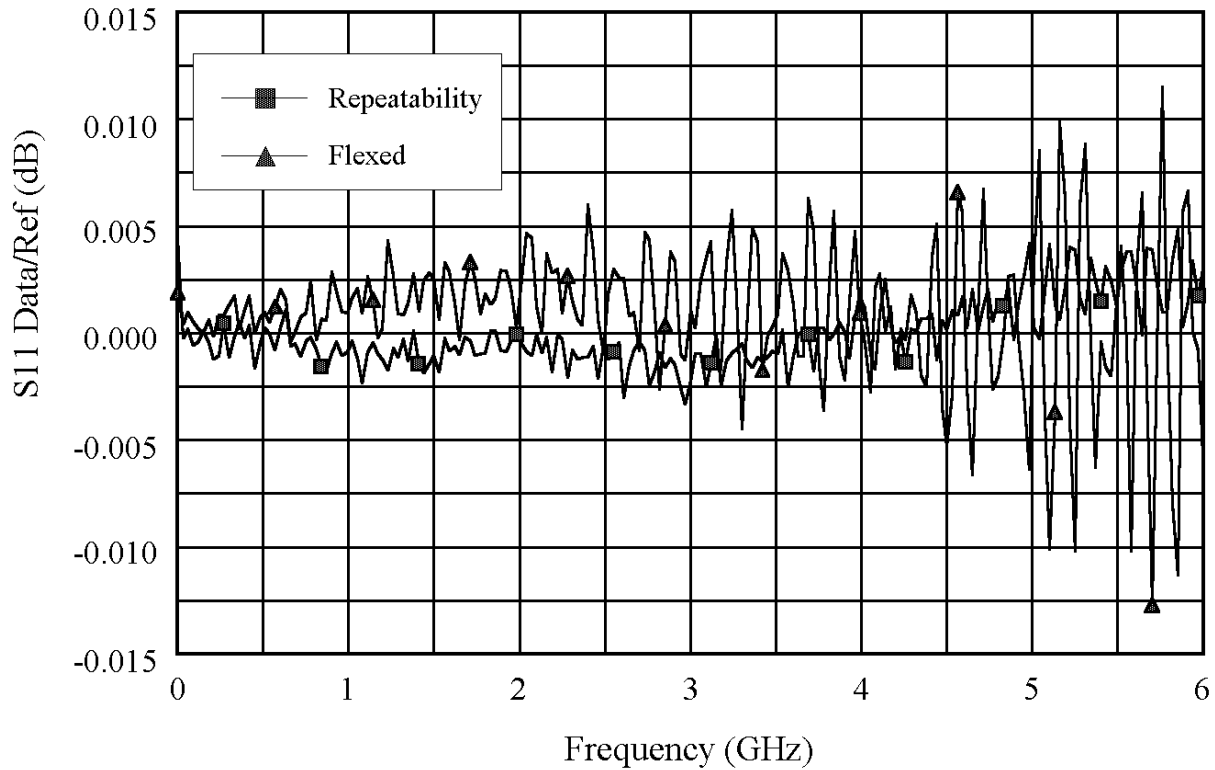

Graphic 2 and Graphic 3 demonstrate the concepts useful in determining cable transmission stability. A short is connected to the free end. The DATA/MEM feature provides an indication of the two-way cable transmission stability. The one-way transmission magnitude stability is determined by dividing the two-way magnitude measurement by two before it is converted to linear. A 0.013-dB peak on the chart yields transmission magnitude stability estimated as  $10^{(0.013/40)} - 1$  or 0.00075. The one-way transmission phase stability is determined by dividing the two-way phase measurement by two.

#### Graphic 3

## Cable Stability with Short Connected

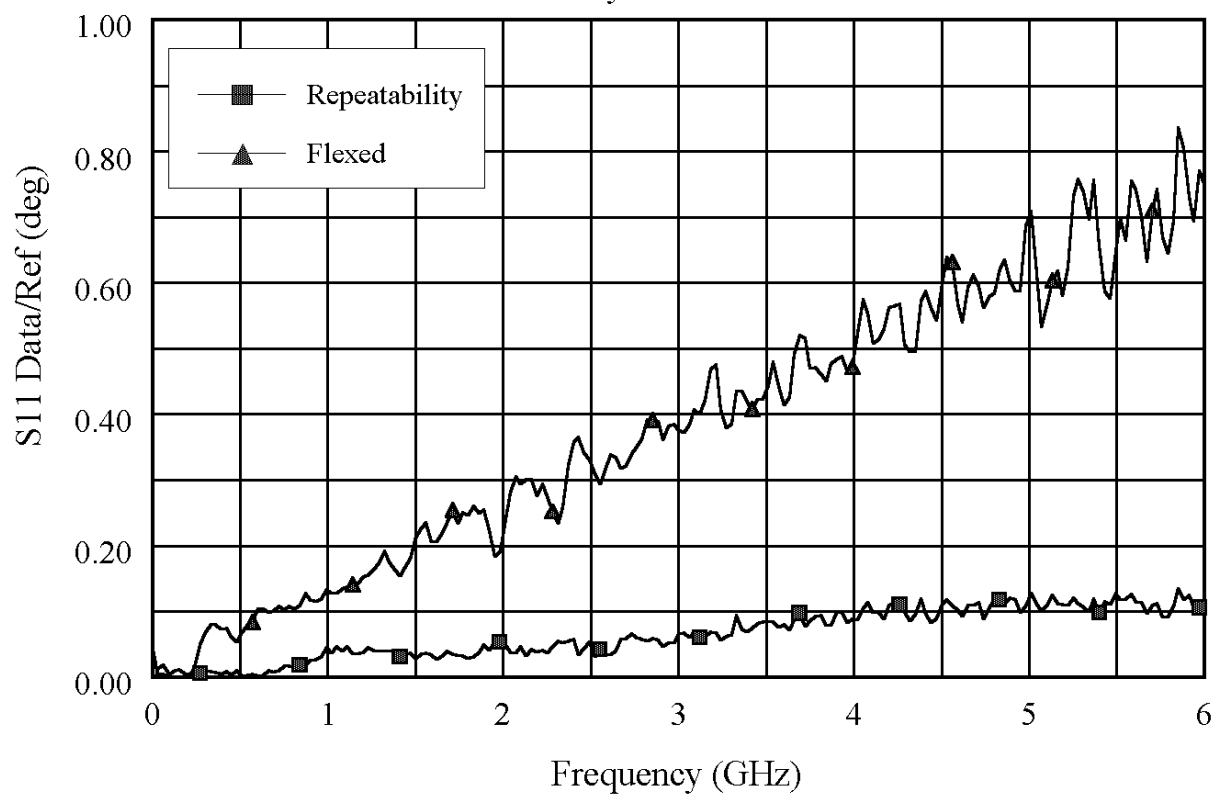

Cable movement often has a much larger effect on phase measurements than magnitude measurements.

### See Also

[Measurement Errors](#)

[What is Measurement Calibration?](#)

[Why is Calibration Necessary?](#)

## Diagnostic Tools and Adjustments

---

The following programs and utilities are available to help you keep your PNA at peak performance.

[10 MHz Reference Frequency Adjustment](#)

[3.8 GHz Frequency Adjustment](#)

[LO Power Adjustment](#)

[Offset LO Power Adjustment](#)

[Operators Check](#)

[Option H11 Verification](#)

[Phase-Lock IF Gain Adjustment](#)

[Receiver Calibration](#)

[Receiver Display](#)

[Serial Bus](#)

[Source Calibration](#)

[System Verification](#)

## Default EE Data

---

The default EE adjustment is to be performed by factory or service personnel ONLY. Therefore, it is not accessible from the PNA adjustments menu.

A password is required to begin using this utility. This utility is only valid on the N5230A and N5340A. Normally, this adjustment should not need to be performed.

This adjustment will default the contents of EE values stored for the following 5 assemblies:

1. Source Synthesizer
2. LO Synthesizer
3. Source Multiplier
4. LO Multiplier
5. MA26 - Modulator Amplifier (if present)

Each assembly can be individually defaulted as needed with predefined default values. An adjustment routine is also provided in case the default values are not sufficient.

If the adjustment routine is used, a power sensor (26.5GHz max) must be connected to various outputs depending upon the board assembly being adjusted.

A verification routine is provided to check the validity of the current settings.

## Preventing PNA Hard Drive Problems - CRITICAL

---

The leading cause of PNA failures is problems with the PNA Hard Disk Drive (HDD). These problems are usually preventable, and in many cases, recoverable (see [Recovering from PNA HDD Problems](#)). The following could save you weeks of downtime and the cost of replacing your PNA HDD.

### Do NOT Modify or Reconfigure the Operating System

The Microsoft Windows operating system has been modified and optimized by Agilent to improve the performance of the PNA.

- Do NOT install a standard version of the Windows operating system on the PNA.
- Do NOT change advanced performance settings or group policies.
- Do NOT add or delete any hard disk drive partitions on the PNA.
- Do NOT delete the Agilent user account.
- Do NOT modify any of the Agilent software registry entries.

### Install Antivirus Protection

The PNA does **NOT** have antivirus protection when shipped. Use of an antivirus program is strongly recommended if you connect the PNA to the Internet.

In addition, the use of a firewall could help to protect the PNA from viruses. However, some firewalls could limit DCOM connectivity of the PNA.

### Install Windows Critical Updates

The PNA is always shipped with the latest service packs and critical updates that were available at the time that the PNA is produced. We recommend that you maintain the latest available protection for your PNA by automatically accepting and installing the latest critical security patches from the Microsoft Windows Update website: <http://windowsupdate.microsoft.com>

### Use AgileUpdate

If your PNA is connected to the Internet, use the [AgileUpdate](#) to obtain the latest firmware. On the PNA, click **System, Service, AgileUpdate** to automatically update your firmware to the current revision.

If your PNA is NOT connected to the Internet, you must update firmware using a CDROM or pen drive. When updating, NEVER skip a major PNA firmware revision. For example, to update from A.02.xx to A.04.xx, first install any version of A.03.xx, then update to A.04.xx.

### Remove Power from the PNA ONLY when the Power Button is Yellow

Unplugging the power cord, or otherwise removing power when the power button is green, can damage the PNA HDD. [Learn more about powering the PNA ON and OFF.](#)

### Having PNA HDD Problems?

If you are experiencing problems which may be caused by a faulty PNA HDD, please see [Recovering from PNA HDD Problems](#).

## Product Support Overview

---

[Troubleshoot the PNA](#)

[Specifications](#)

[About Error Messages](#)

[Analyzer Accessories](#)

[82357A USB/GPIB Interface](#)

[Firmware Upgrade](#)

[PNA Configurations and Options](#)

[Diagnostic Tools and Adjustments](#)

[Other Resources](#)

[Technical Support](#)

[Instrument Calibration](#)

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

---



## Tutorials

---

[Network Analyzer Basics \(multimedia\)](#)

[Connector Care](#)

[Electrostatic Discharge \(ESD\) Protection](#)

[Time Domain Measurements](#)

## List of Device Measurements

[Absolute Output Power](#)

[AM-PM Conversion](#)

[Complex Impedance](#)

[Deviation from Linear Phase](#)

[Gain and Flatness](#)

[Gain Compression](#)

[Group Delay](#)

[High Power Components](#)

[Impedance Matching Model \(animation\)](#)

[Phase Measurements](#)

[Reverse Isolation](#)

[Reflection Measurements](#)

[Reflected Waves Model \(animation\)](#)

---

**Caution:** Avoid expensive repairs to your PNA. Read [Electrostatic Discharge Protection](#).

---



## COM Example Programs

---

### Calibrations

|                                                                     |              |
|---------------------------------------------------------------------|--------------|
| <u>Perform a Guided Cal</u>                                         | VBScript     |
| <u>Perform an ECal</u>                                              | VBScript     |
| <u>Perform an ECAL Confidence Check</u>                             | Visual Basic |
| <u>Perform an Unknown Thru or TRL Cal (apply a Delta Match Cal)</u> | VBScript     |
| <u>Perform Global Delta Match Cal</u>                               | VBScript     |
| <u>Reading Cal Set Data</u>                                         | VBScript     |
| <u>Writing Cal Set Data</u>                                         | VBScript     |
| <u>Perform a Source Power Cal using COM</u>                         | VBScript     |
| <u>Upload a Source Power Cal using COM</u>                          | VBScript     |

### FCA

|                                                             |              |
|-------------------------------------------------------------|--------------|
| <u>Create Mixer Measurement and Perform SMC Calibration</u> | Visual Basic |
| <u>Create Mixer Measurement and Perform VMC Calibration</u> | VBScript     |
| <u>Create an SMC Fixed Output Measurement</u>               | Visual Basic |

### Miscellaneous

|                                        |              |
|----------------------------------------|--------------|
| <u>E5091 Testset Control</u>           |              |
| <u>Getting Trace Data from the PNA</u> | Visual Basic |
| <u>Upload Segment Table</u>            | Visual Basic |
| <u>Create a Balanced Measurement</u>   | VBScript     |
| <u>Create a Pulsed Measurement</u>     | Visual Basic |
| <u>Limit Line Testing</u>              | Visual Basic |
| <u>Events Example</u>                  | Visual Basic |

See more PNA programming information and examples at: <http://na.tm.agilent.com/pna/programming/>

## Create a Balanced Measurement using COM

---

The following program creates several Balanced measurements in separate windows, generates markers, calculates statistics, and sets limit lines and queries results.

**Note:** By their nature, balanced measurements are extremely sensitive to phase differences between the two RF paths that make up the balanced port, especially at higher frequencies. A good calibration (not performed in this example) is critical to achieving good balanced measurement results.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as BalancedCOM.vbs. [Learn how to setup and run the macro.](#)

```
' PNA application object
Dim app

' Channel 1 object
Dim chan1

' start of marker/limit testing range
Dim minTestStimulus

' end of marker/limit testing range
Dim maxTestStimulus

' Set to true if you want additional balanced measurements.
Dim AdditionalMeasurements
AdditionalMeasurements = 1

' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
' Preset the instrument
app.Reset
' Get the Channel 1 object
Set chan1 = app.Channels(1)
' Stop data taking for now.
chan1.Hold true
' Set up the start / stop frequency for Channel 1 sweep.
MHZ = 1000000
GHZ = 1000*MHZ
chan1.StartFrequency = 10 *MHZ
chan1.StopFrequency = 1 *GHZ
chan1.NumberOfPoints = 801
' Define our test frequency range
minTestStimulus = 100*MHZ
maxTestStimulus = 900*MHZ
' This example uses DUT topology Bal-Bal -
' a DUT with a balanced input and balanced output.
'
' Port mapping for our DUT:
' logical port 1 = physical ports 1 and 4
' logical port 2 = physical ports 2 and 3
' The default is:
' logical port 1 = physical ports 1 and 2
' logical port 2 = physical ports 3 and 4
```

```

'
' logical 1 logical 2
'
' 1 -----| |----- 2 +
' | |
' | DUT |
' | |
' 4 -----| |----- 3 -
'
chan1.BalancedTopology.SetBBPorts 1, 4, 2, 3

' Now we create some Bal-Bal measurements.
' By creating Bal-Bal measurements ("BBAL:..."),
' the channel is set to Bal-Bal topology,
' so it is not necessary to do this explicitly
' with the BalancedTopology.DUTTopology command.
' We do it here just for clarity:

chan1.BalancedTopology.DUTTopology = 2
' 0 == SE-Bal, 1 == SE-SE-Bal, 2 == Bal-Bal

' Create four windows, each showing one category of balanced measurement:
' Create Forward Transmission Measurements in Bal-Bal topology on Channel 1, window
1

' differential mode transmission
app.CreateMeasurement 1, "BBAL:SDD21",1,1
Set sdd21_1 = app.ActiveMeasurement

' differential to common mode conversion
app.CreateMeasurement 1, "BBAL:SCD21",1,1
Set scd21_1 = app.ActiveMeasurement

' common to differential mode conversion
app.CreateMeasurement 1, "BBAL:SDC21",1,1
Set sdc21_1 = app.ActiveMeasurement

' common mode transmission
app.CreateMeasurement 1, "BBAL:SCC21",1,1
Set scc21_1 = app.ActiveMeasurement

' Optionally create some additional measurements
If AdditionalMeasurements Then

' Create (logical) Port 1 reflection measurements, channel 1, window 2
app.CreateMeasurement 1, "BBAL:SDD11",1,2 ' differential mode reflection
app.CreateMeasurement 1, "BBAL:SDC11",1,2 ' C to D mode conversion reflection
app.CreateMeasurement 1, "BBAL:SCD11",1,2 ' D to C mode conversion reflection
app.CreateMeasurement 1, "BBAL:SCC11",1,2 ' common mode reflection

' Create Reverse Transmission Measurements, channel 1, window 3
app.CreateMeasurement 1, "BBAL:SDD12",1,3 ' differential mode transmission
app.CreateMeasurement 1, "BBAL:SCD12",1,3 ' differential to common mode conversion
app.CreateMeasurement 1, "BBAL:SDC12",1,3 ' common to differential mode conversion
app.CreateMeasurement 1, "BBAL:SCC12",1,3 ' common mode transmission

' Create (logical) Port 2 reflection measurements in window 4
app.CreateMeasurement 1, "BBAL:SDD22",1,4 ' differential mode reflection
app.CreateMeasurement 1, "BBAL:SDC22",1,4 ' C to D mode conversion reflection

```

```

app.CreateMeasurement 1, "BBAL:SCD22",1,4 ' D to C mode conversion reflection
app.CreateMeasurement 1, "BBAL:SCC22",1,4 ' common mode reflection
End If

' Set up some limit lines to verify a minimum differential insertion loss
sdd21_1.LimitTest(1).BeginStimulus = minTestStimulus
sdd21_1.LimitTest(1).EndStimulus = maxTestStimulus
sdd21_1.LimitTest(1).BeginResponse = -2
sdd21_1.LimitTest(1).EndResponse = -2
sdd21_1.LimitTest(1).Type = 2 ' minimum limit
sdd21_1.LimitTest.State = 1
' Limit lines for maximum common mode to differential conversion
sdc21_1.LimitTest(1).BeginStimulus = minTestStimulus
sdc21_1.LimitTest(1).EndStimulus = maxTestStimulus
sdc21_1.LimitTest(1).BeginResponse = -20
sdc21_1.LimitTest(1).EndResponse = -20
sdc21_1.LimitTest(1).Type = 1 ' maximum limit
sdc21_1.LimitTest.State = 1
' Take a (synchronous) single sweep on channel 1
chan1.Single true

' Show differential forward transmission statistics.
sdd21_1.ShowStatistics = true

' Set up user range 1 to limit marker's search range.
chan1.UserRangeMin(0,1) = minTestStimulus
chan1.UserRangeMax(0,1) = maxTestStimulus

' Find/Show max common mode to differential conversion, and read back the frequency.
sdc21_1.MarkerState(1) = true
' Set marker 1 to use user range 1
sdc21_1.Marker(1).UserRange = 1
sdc21_1.Marker(1).SearchMax

' Find/Show max differential mode insertion loss, and read back the frequency.
sdd21_1.MarkerState(1) = true
' Set marker 1 to use user range 1
sdd21_1.Marker(1).UserRange = 1
sdd21_1.Marker(1).SearchMin
If sdd21_1.LimitTestFailed Then
Wscript.Echo "Differential insertion loss failed: " & sdd21_1.Marker(1).Stimulus
/MHz & "MHz, " & _sdd21_1.Marker(1).Value(1) & " dB"
End If

If sdc21_1.LimitTestFailed Then
Wscript.Echo "Common to differential conversion failed: " &
sdc21_1.Marker(1).Stimulus/MHz & "MHz, " & _sdc21_1.Marker(1).Value(1) & " dB"
End If

```

## C++ Example

---

The following example uses the smart pointer created by Microsoft Visual Studio. The calls to CoInitialize and CoUninitialize open and close the COM libraries.

Also notice that the pointers local to the main routine are explicitly released. When smart pointers go out of scope, they will perform this duty implicitly. However, we are calling CoUninitialize before they have the chance to be destroyed, so we are obliged to release them.

---


```
// An example program to illustrate the use of #import to bind to the
// PNA type library.
//

#ifdef _UNICODE
#define _UNICODE
#endif

#include "stdafx.h"
#include "stdio.h"
#include "math.h"

////////////////////////////////////
// import the network analyzer type library
////////////////////////////////////
#import "C:\Program Files\Common Files\Agilent\Pna\835x.tlb" no_namespace,
named_guids
////////////////////////////////////
// include the error definitions for the PNA so we can implement
// error handling.
////////////////////////////////////
#include "C:\Program Files\Common Files\Agilent\Pna\errorsystemmessage.h"

IApplicationPtr pNA; // top level application pointer
float fScalarData [1601]; // global buffer for data retrieval
float fScalarData2[1601];

DWORD dwCookie;

////////////////////////////////////
// SetupChannel:
//
// input: pointer to the channel
//
// function: sets properties on the channel
////////////////////////////////////
void SetupChannel(IChannelPtr pChannel)
{
 pChannel->put_StartFrequency(1.2E9);
 pChannel->put_StopFrequency (4.2E9);
 pChannel->put_NumberOfPoints (201);
}

////////////////////////////////////
// AcquireData:
```



```

BSTR param;
pMeas->get_Parameter(¶m);
swprintf(msg,L"Review %s data",param);
MessageBox(NULL,msg,L"User Message",0);
::SysFreeString(param);
}
//
// PutData:
//
// input: pointer to the Measurement object
//
// function: writes data to the measurment's raw data
// buffer
//
void PutData(IMeasurementPtr pMeas)
{
 IArrayTransferPtr pDataTransfer;
 pDataTransfer = pMeas;
 long numVals = 201;

 if(pDataTransfer){
 NAComplex* pComplex = new NAComplex[numVals];

 pComplex[0].Im = 0;
 pComplex[0].Re = 1;
 for (int i = 1; i < numVals; i++)
 {
 pComplex[i].Im = (float)sin(i)/i;
 pComplex[i].Re = (float)cos(i)/i;
 }

 pDataTransfer->putNAComplex(naRawData, numVals, pComplex, naDataFormat_Polar);
 delete [] pComplex;
 }
}

//
// printError
//
void printError(HRESULT hr)
{
 BSTR text;

 hr = pNA->get_MessageText ((NAEventID) hr, &text);
 MessageBox(NULL,text,L"Network Analyzer error",0);
 ::SysFreeString(text);
}

//
// main
//
int main(int argc, char* argv[])
{
 HRESULT hr;
 const long channel1 = 1;

```

```

const long window1 = 1;
const long srcport = 1;
IMeasurementPtr pMeasurement;
IChannelPtr pChannel;

// initialize COM libraries
CoInitialize(NULL);

try {
pNA = IApplicationPtr("AgilentPNA835x.Application.1");

pNA->put_Visible(TRUE);
pNA->Reset();

pNA->CreateMeasurement (channel1, "S21",srcport, 3);
hr = pNA->get_ActiveChannel(&pChannel);

if (SUCCEEDED (hr))
{
SetupChannel(pChannel);
AcquireData(pChannel);
}

hr= pNA->get_ActiveMeasurement(&pMeasurement);
if (SUCCEEDED(hr))
{
pMeasurement->put_Format(naDataFormat_Polar);
ReadScalarData(pMeasurement);
ReadComplexData(pMeasurement);
PutData(pMeasurement);
}
if (FAILED(hr))
{
printError(hr);
}

// make sure to release the remaining pointers
// before calling CoUninitialize

pMeasurement.Release();
pChannel.Release();
pNA.Release();
}
catch (_com_error err)
{
printError(err.Error());
}

CoUninitialize();
return 0;
}

```



## E5091Testset Control

---

The following VB Script example exercises the COM commands used to control the E5091A testset.

For a description of each command, see [E5091Testsets collection](#).

```
Sub Main()
Set pna = CreateObject("AgilentPNA835x.Application")
Dim testsets As E5091Testsets
Set testsets = pna.E5091Testsets
Dim tset1 As E5091Testset
Set tset1 = testsets(1)
tset1.OutputPort(1, 3) = naE5091PortR2
tset1.ControlLines(1) = 5
tset1.ShowProperties = True
tset1.Enabled = True
MsgBox tset1.ID
MsgBox tset1.Enabled
MsgBox tset1.ShowProperties
' NumberOfPorts property returns 0 when testset not connected
MsgBox tset1.NumberOfPorts
MsgBox tset1.OutputPort(1, 3)
MsgBox tset1.ControlLines(1)

Dim tset2 As E5091Testset
Set tset2 = testsets(2)
tset2.Enabled = True
tset2.ShowProperties = True
MsgBox tset2.Enabled
MsgBox tset2.ShowProperties
End Sub
```

## Perform an ECal using COM

---

This example uses the [GuidedCalibration](#) interface to perform a 2-port ECal calibration.

Learn more about [Reading and Writing Calibration data using COM](#).

### See Other COM Example Programs

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save on the PNA hard drive as ECal.vbs. [Learn how to setup and run the macro](#).

```
Set pna = CreateObject("AgilentPNA835x.Application")
Set calMgr = pna.GetCalManager
Set guidedCal = calMgr.GuidedCalibration
Set chan = pna.ActiveChannel
chanNum = chan.ChannelNumber
' Initialize guided cal to be performed on the active channel.
' The boolean argument of True indicates to create a new calset
guidedCal.Initialize chanNum, True
' To perform 3-port cal, Uncomment the following
' Then comment the 2-port cal

' Do 2-port cal
TwoPortGuidedCal

' Do 3-port cal
' ThreePortGuidedCal

Sub TwoPortGuidedCal()
'Change the following to match the connectors on your ECal module
guidedCal.ConnectorType(1) = "APC 3.5 female"
guidedCal.ConnectorType(2) = "APC 3.5 female"
For i = 3 To pna.NumberOfPorts
guidedCal.ConnectorType(i) = "Not used"
Next
value = MsgBox("Connectors defined for Ports 1 and 2")
' Select the ECal module for each port being calibrated.
' Replace N4691-60004 with your own ECAL model followed by 'ECal'.
' Your ECal module must already be connected to a PNA USB port.

guidedCal.CalKitType(1) = "85092-60010 ECal"
guidedCal.CalKitType(2) = "85092-60010 ECal"

value = MsgBox("ECal Module defined for Ports 1 and 2")
' Initiate the calibration and query the number of steps
numSteps = guidedCal.GenerateSteps
' Measure the standards, compute and apply the cal
MeasureAndComplete(numSteps)
End Sub

Sub ThreePortGuidedCal()
'Change the following to match the connectors on your ECal module
guidedCal.ConnectorType(1) = "APC 3.5 female"
```

```

guidedCal.ConnectorType(2) = "APC 3.5 female"
guidedCal.ConnectorType(3) = "APC 3.5 female"

' Select the ECal module for each port being calibrated.
' Replace N4691-60003 with your own ECAL model followed by 'ECal'.
' Your ECal module must already be connected to a PNA USB port.
guidedCal.CalKitType(1) = "N4431-60003 ECal"
guidedCal.CalKitType(2) = "N4431-60003 ECal"
guidedCal.CalKitType(3) = "N4431-60003 ECal"

value = MsgBox("Cal kits defined for Ports 1 to 3")
' Initiate the calibration
numSteps = guidedCal.GenerateSteps
' Measure the standards, compute and apply the cal
MeasureAndComplete(numSteps)
End Sub

Sub MeasureAndComplete(ByVal numSteps)
value = MsgBox("Number of steps is " + CStr(numSteps))
' Measure the standards
For i = 1 To numSteps
step = "Step " + CStr(i) + " of " + CStr(numSteps)
strPrompt = guidedCal.GetStepDescription(i)
value = MsgBox(strPrompt, vbOKOnly, step)
guidedCal.AcquireStep i
Next

' Conclude the calibration
guidedCal.GenerateErrorTerms
MsgBox ("Cal is done!")
End Sub

```

## Perform an Unguided Cal using COM

---

This example uses the [ICalibrator](#) interface to do the following:

- perform a two port calibration
- retrieve the error term data
- retrieve the standard data (cal acquisition data)

Learn more about [Reading and Writing Calibration data using COM](#).

### See Other COM Example Programs

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save on the PNA hard drive as Calibrate.vbs. [Learn how to setup and run the macro](#).

```
dim pna
' To run from an external PC, substitute your PNA Name and use the following
command.
' set pna = CreateObject("AgilentPNA835x.Application", "PNA Name")
set pna = CreateObject("AgilentPNA835x.Application")
dim calibrator
set calibrator=pna.activechannel.calibrator

wscript.echo "setcalinfo for two port cal"
calibrator.setcalinfo 5,1, 2

' only have one set of standards
calibrator.Simultaneous2PortAcquisition = false

'first acquire forward reflection standards, then reverse
dim p
for p = 1 to 2

if (p = 1) then
calibrator.AcquisitionDirection = 0
else
calibrator.AcquisitionDirection = 1
end if

wscript.echo "connect open to port ", p
calibrator.acquirecalstandard 1

wscript.echo "connect short to port ", p
calibrator.acquirecalstandard 2

wscript.echo "connect load to port ", p
calibrator.acquirecalstandard 3

next
```

```

wscript.echo "connect a thru1"
calibrator.acquirecalstandard 4

'Optional - perform isolation
wscript.echo "connect loads to both ports"
calibrator.acquirecalstandard 5

wscript.echo "calculating"
calibrator.CalculateErrorCoefficients

'Calibration complete
' Now read error terms and standard data

dim termName
termName= Array("Directivity","SourceMatch","ReflectionTracking")
dim vardata

' iterate over error terms
dim t
for t = 0 to 2 ' per error term
for p = 1 to 2 ' per port
wscript.echo "Requesting ",termName(t),p,p
vardata = calibrator.GetErrorTerm(t, p, p)
next
next

' now get the path terms: iterator each one request
termName = Array("Isolation", "LoadMatch", "TransmissionTracking")
for t = 0 to 2

wscript.echo "Requesting Forward term",termName(t),1,2
vardata = calibrator.GetErrorTerm(t, 1,2)
wscript.echo "Requesting Reverse Term",termName(t),2,1
vardata = calibrator.GetErrorTerm(t, 2,1)
next

dim stdname
stdname= Array("", "Open", "Short", "Load", "Thru", "Isolation")

' iterate over the port standards
for t = 1 to 3
for p = 1 to 2
' request the standard term for each port of interest
wscript.echo "Requesting",stdname(t),p,p

vardata = calibrator.GetStandard(t, p, p)
next
next

' now get the path standards: iterator each one request
for t = 4 to 5

wscript.echo "Requesting Forward",stdname(t),1,2
vardata = calibrator.GetStandard(t, 1,2)

wscript.echo "Requesting Reverse",stdname(t),2,1

```

```
vardata = calibrator.GetStandard(t, 2,1)
```

```
next
```

## Perform an Unknown Thru or TRL Cal

---

The following program performs either a 2-port SOLT Unknown Thru Cal or a 2-port TRL Cal. The 85052C Cal Kit used in this program contains both types of standards. This program can be run on 2-port or 4-port PNAs. When run on a 4-port PNA, which does not have a reference receiver per port, a [Delta Match Cal](#) is required. See example of Delta Match Cal.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Unknown.vbs. [Learn how to setup and run the macro.](#)

```
PerformUnknownThruOrTRLCal
Sub PerformUnknownThruOrTRLCal()
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
' Get the cal manager object
Set calMgr = app.GetCalManager
' Get the guided cal object
Set guidedCal = calMgr.GuidedCalibration
Set chan = app.ActiveChannel
chanNum = chan.ChannelNumber

' Initialize guided cal to be performed on the active channel.
' The boolean argument of True specifies the creation of a new calset
' for storing the new calibration.
guidedCal.Initialize chanNum, True

' Specify connectors for Ports 1 and 2
guidedCal.ConnectorType(1) = "APC 3.5 female"
guidedCal.ConnectorType(2) = "APC 3.5 male"

' If your PNA has more than 2 ports, uncomment one or both of
' these next two lines, to explicitly specify this is
' just a 2-port cal.
'guidedCal.ConnectorType(3) = "Not used"
'guidedCal.ConnectorType(4) = "Not used"

' Specify cal kit for Ports 1 and 2
guidedCal.CalKitType(1) = "85052C"
guidedCal.CalKitType(2) = "85052C"

' Since the 85052C cal kit contains SOLT standards and also TRL
' standards, this next line determines whether the cal becomes
' unknown thru (SOLT), or TRL.
' Specify cal method
guidedCal.ThruCalMethod = 4 ' 4 = naUnknownThru

' To set up the cal as TRL, comment the previous line and uncomment this next line
'guidedCal.ThruCalMethod = 6 ' 6 = naTRL

' Initiate the calibration and query the number of steps
numSteps = guidedCal.GenerateSteps
MsgBox "Number of steps is " + CStr(numSteps)

' Query the list of ports that need delta match
portList = guidedCal.PortsNeedingDeltaMatch
```

```

' If portList contains just one element and it's value is 0, then that indicates
' none of the ports being calibrated require delta match data.
' If each testport on the PNA has it's own reference receiver (R channel),
' then delta match is never needed, so portList will always be just 0.
lowerBound = LBound(portList)
If (UBound(portList) <> lowerBound) Or (portList(lowerBound) <> 0) Then
 ' Delta match data is required for at least one port.
 ' For this example, we assume a Global Delta Match Cal has previously been
 ' performed so the Global Delta Match CalSet exists.
 ' Supplying an empty string to ApplyDeltaMatchFromCalSet indicates to use
 ' the Global Delta Match CalSet.
 MsgBox "here"
 guidedCal.ApplyDeltaMatchFromCalSet ""
End If

' Measure the standards
For i = 1 To numSteps
 step = "Step " + CStr(i) + " of " + CStr(numSteps)
 strPrompt = guidedCal.GetStepDescription(i)
 retVal = MsgBox(strPrompt, vbOKCancel, step)
 If retVal = vbCancel Then Exit Sub
 guidedCal.AcquireStep i
Next

' Conclude the calibration
guidedCal.GenerateErrorTerms
MsgBox "Cal is done!"

End Sub

```



## Perform a Guided Calibration using COM

---

This example uses the [GuidedCalibration](#) interface to perform either a 2-port or 4-port calibration.

Learn more about [Reading and Writing Calibration data using COM](#).

### See Other COM Example Programs

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save on the PNA hard drive as Calibrate.vbs. [Learn how to setup and run the macro](#).

```
Set pna = CreateObject("AgilentPNA835x.Application")
Set calMgr = pna.GetCalManager
Set guidedCal = calMgr.GuidedCalibration
Set chan = pna.ActiveChannel
chanNum = chan.ChannelNumber
' Initialize guided cal to be performed on the active channel.
' The boolean argument of True indicates to store the cal only
' in the channel's calibration register. If instead you wish
' to create a new calset that the new cal will get stored to,
' comment out this next line and uncomment the three lines below it.
guidedCal.Initialize chanNum, True
'Set calset = calMgr.CreateCalSet(chanNum)
'chan.SelectCalSet calset.GetGUID, True
'guidedCal.Initialize chanNum, False

' To perform 2-port cal, Uncomment the following
' Then comment the 4-port cal

' Do 2-port cal
' TwoPortGuidedCal

' Do 4-port cal
FourPortGuidedCal

Sub TwoPortGuidedCal()
' Select the connectors
guidedCal.ConnectorType(1) = "APC 3.5 female"
guidedCal.ConnectorType(2) = "APC 3.5 male"
For i = 3 To pna.NumberOfPorts
 guidedCal.ConnectorType(i) = "Not used"
Next
value = MsgBox("Connectors defined for Ports 1 and 2")
' Select the Cal Kit for each port being calibrated.
guidedCal.CalKitType(1) = "85052D"
guidedCal.CalKitType(2) = "85052D"
' To use an ECal module instead, comment out the above two lines
' and uncomment the following two lines.
' Replace N4691-60004 with your own ECAL model followed by 'ECal'.
' Your ECal module must already be connected to a PNA USB port.
'guidedCal.CalKitType(1) = "N4691-60004 ECal"
```

```

'guidedCal.CalKitType(2) = "N4691-60004 ECal"
value = MsgBox("Cal kits defined for Ports 1 and 2")
' Initiate the calibration and query the number of steps
numSteps = guidedCal.GenerateSteps
' Measure the standards, compute and apply the cal
MeasureAndComplete(numSteps)
End Sub

Sub FourPortGuidedCal()
' Select the connectors
guidedCal.ConnectorType(1) = "APC 3.5 female"
guidedCal.ConnectorType(2) = "APC 3.5 female"
guidedCal.ConnectorType(3) = "APC 3.5 female"
guidedCal.ConnectorType(4) = "APC 3.5 female"
' If a PNA which has more than 4 ports
For i = 5 To pna.NumberOfPorts
 guidedCal.ConnectorType(i) = "Not used"
Next
value = MsgBox("Connectors defined for Ports 1 to 4")
' Select the Cal Kit for each port being calibrated.
guidedCal.CalKitType(1) = "85052D"
guidedCal.CalKitType(2) = "85052D"
guidedCal.CalKitType(3) = "85052D"
guidedCal.CalKitType(4) = "85052D"
' To use an ECal module instead, comment out the above four lines
' and uncomment the following four lines.
' Replace N4691-60003 with your own ECAL model followed by 'ECal'.
' Your ECal module must already be connected to a PNA USB port.
'guidedCal.CalKitType(1) = "N4431-60003 ECal"
'guidedCal.CalKitType(2) = "N4431-60003 ECal"
'guidedCal.CalKitType(3) = "N4431-60003 ECal"
'guidedCal.CalKitType(4) = "N4431-60003 ECal"
value = MsgBox("Cal kits defined for Ports 1 to 4")
' Initiate the calibration
guidedCal.GenerateSteps
' If your selected cal kit is not a 4-port ECal module which can
' mate to all 4 ports at once, then you may want to choose which
' thru connections to measure for the cal. You must measure at
' least 3 different thru paths for a 4-port cal (for greatest
' accuracy you can choose to measure a thru connection for all 6
' pairings of the 4 ports). If you omit this command, the default
' is to measure from port 1 to port 2, port 1 to port 3, and
' port 1 to port 4. For this example we select to measure
' from port 1 to port 2, port 2 to port 3, and port 2 to port 4.
portList = Array(1,2,2,3,2,4)
guidedCal.ThruPortList = portList
' Re-generate the connection steps to account for the thru changes
numSteps = guidedCal.GenerateSteps
' Measure the standards, compute and apply the cal
MeasureAndComplete(numSteps)
End Sub

Sub MeasureAndComplete(ByVal numSteps)
value = MsgBox("Number of steps is " + CStr(numSteps))
' Measure the standards
For i = 1 To numSteps
 step = "Step " + CStr(i) + " of " + CStr(numSteps)

```

```
strPrompt = guidedCal.GetStepDescription(i)
value = MsgBox(strPrompt, vbOKOnly, step)
guidedCal.AcquireStep i
Next

' Conclude the calibration
guidedCal.GenerateErrorTerms
MsgBox ("Cal is done!")
End Sub
```

## Perform Global Delta Match Cal

---

The following program performs a [Global Delta Match Calibration](#). This is required when performing an Unknown Thru Cal or TRL Cal on PNAs without a reference receiver for each test port. [See example of Unknown Thru or TRL Cal](#).

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Delta.vbs. [Learn how to setup and run the macro](#).

```
Sub PerformGlobalDeltaMatchCal()
Set pna = CreateObject("AgilentPNA835x.Application")
Set scpi = pna.ScpiStringParser

' Initiate a Global Delta Match calibration, choosing connector and cal kit
scpi.Parse "SENS:CORR:COLL:GUID:DMAT 'APC 3.5 female', '85033D/E'"

' Query the number of calibration steps
retStr = scpi.Parse("SENS:CORR:COLL:GUID:STEP?")
numSteps = CInt(retStr)

' Measure the cal standards
For i = 1 To numSteps
 prompt = scpi.Parse("SENS:CORR:COLL:GUID:DESC? " & CStr(i))
 retVal = MsgBox(prompt, vbOKCancel)
 If retVal = vbCancel Then Exit Sub
 retStr = scpi.Parse("SENS:CORR:COLL:GUID:ACQ STAN" & CStr(i) & ";*OPC?")
Next

' Compute the error coefficients and save the cal to Global Delta Match CalSet
scpi.Parse "SENS:CORR:COLL:GUID:SAVE"
MsgBox "Cal is done!"
End Sub
```

## Writing Cal Set Data using COM

---

This example creates a Cal Set and then writes data to the Cal Set.

Learn more about [Reading and Writing Calibration data using COM](#).

Learn more about [Cal Sets](#).

### See Other COM Example Programs

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save on the PNA hard drive as CalSetsWrite.vbs. [Learn how to setup and run the macro](#).


```
dim pna
dim v
Set pna=CreateObject("AgilentPNA835x.Application")
InitPhonyData
PutPhonyData
' This sub creates phony data
Sub InitPhonyData()
Dim i
Dim numpts
wscript.echo "init phony"
numpts = pna.ActiveChannel.NumberOfPoints
ReDim v(numpts - 1, 1)
For i = 0 To numpts - 1
v(i, 0) = i
v(i, 1) = 0
Next
End Sub

' This sub creates a Cal Set, then writes the phony data to it
Sub PutPhonyData()
Dim cmgr
Dim cset
wscript.echo "putphony"
Set cmgr = pna.GetCalManager
Set cset = cmgr.CreateCalSet(1)
cset.OpenCalSet naCalType_OnePort, 1
const directivity = 0
const sourcematch=1
const reflectiontracking =2
cset.putErrorTerm directivity,1, 1, v
cset.putErrorTerm sourcematch,1, 1, v
cset.putErrorTerm reflectiontracking ,1, 1, v
cset.CloseCalSet
cset.Description = "Phony One Port"
cset.save
End Sub
```

## Control Auxiliary Commands

---

Specifies the settings to remotely control the [Auxilliary IO connector](#).

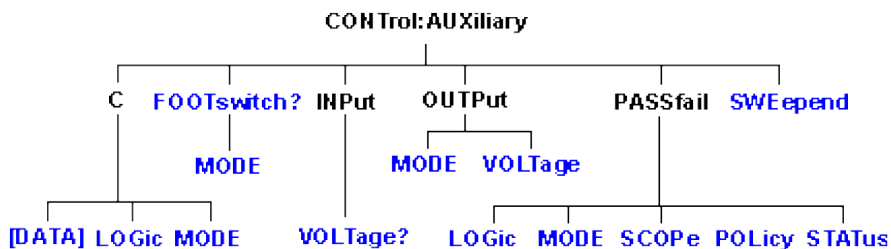

- Click on a **blue** keyword to view the command details.
  - See a [List](#) of all SCPI commands.
  - See a pinout and detailed description of the [Auxilliary IO connector](#).
- 

### CONTROL:AUXiliary:C[:DATA] <num>

(Read-Write) Reads and writes a 4-bit value to Port C on the Aux I/O connector. This port is connected internally to the Handler IO connector. Therefore this command will also affect the state of Port C on the Handler IO

#### Parameters

<num> Data value. Choose any number 0 to 15.

#### Examples

```
CONTROL:AUXiliary:C:DATA 15
```

For Positive Logic Port C lines C0, C1, C2, C3 go High or if in Negative Logic they go Low.

```
CONTROL:AUXiliary:C:DATA?
```

A returned value of 15 when in Positive Logic indicates Port C lines C0, C1, C2, C3 are High, or if in Negative Logic they are Low.

**Query Syntax** CONTROL:AUXiliary:C:DATA?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### CONTROL:AUXiliary:C:LOGic <char>

(Read-Write) Reads and writes the logic mode of Port C on the AUX IO. This port is connected to Port C of the Handler IO connector. Therefore, it will have the same logic setting.

### Parameters

<char> Logic of Port C. Choose from:

**POSitive** - when a value of one is written the associate line goes High.

**NEGative** - when a value of one is written the associate line goes Low.

When Port C is in Output/Write mode, a change in logic causes the output lines to change state immediately. For example, Low levels change to High levels.

When Port C is in Input/Read mode, a change in logic does NOT cause the lines to change, but data read from Port C will reflect the change in logic.

**Examples** `CONT:AUX:C:LOG POS 'Positive logic is applied to Port C data.`

**Query Syntax** `CONTrol:AUXiliary:C:LOGic?`

**Return Type** Character

**Overlapped?** No

**Default** NEGative

---

### CONTrol:AUXiliary:C:MODE <char>

(Read-Write) Sets Port C to read or write mode. This port is connected to Port C of the Handler IO connector. Therefore, it will have the same mode setting.

**NOTE:** When Port C is set to INPut mode, data writes are NOT applied to the lines. MODE must be set to OUTPut mode before writing.

---

### Parameters

<char> INPut - set the port for reading

OUTPut - set the port for writing

**Examples** `CONT:AUX:C:MOD INP 'set Port C to Input Mode for reading.`  
`CONTrol:AUXiliary:C:MODE? 'queries the input/output mode that the port set to.`

**Query Syntax** `CONTrol:AUXiliary:C:MODE?`

**Return Type** Character

**Overlapped?** No

**Default** INPut

---

## CONTRol:AUXiliary:FOOTswitch?

(Read only) Reads the Auxiliary connector Footswitch Input ([pin 20 of the AUX IO connector](#)).

**Examples** `CONT:AUX:FOOT?  
control:auxiliary:footswitch?`

**Return Type** Boolean  
**True (or 1)** = pressed  
**False (or 0)** = released

**Overlapped?** No

**Default** False (0) - Released

---

## CONTRol:AUXiliary:FOOTswitch:MODE <char>

(Read-Write) This command sets the mode of the "FootSwitch In" line on the Auxiliary IO. These mode settings determine what occurs when the footswitch is pressed. Examine your results carefully when using these command modes. Refer to each mode description and associated notes, also see the [FootSwitch In pin description](#) in the Auxiliary IO connector documentation.

### Parameters

<char> **IGNore** - While in this mode any Footswitch presses are ignored.

**SWEep** - While in this mode a Footswitch press will trigger the sweep.

---

NOTE: The instrument must be in Manual Trigger Mode.

**RECall** - While in this mode a Footswitch press will recall an instrument state. When more than one state is available each footswitch press recalls the next state, then starts over from the beginning.

---

NOTE: It's possible to override the current mode with a recalled state. For instance when the current footswitch mode is RECall and the footswitch mode in the recalled state is IGNore the mode will change to IGNore. If this occurs additional footswitch presses will be ignored.

---

**MACRo** - While in this mode a Footswitch press will load and run a macro. When more than one macro are available each successive footswitch press loads and runs the next macro, then starts over from the beginning.

---

NOTE: It's possible to override the current mode when using the MACRo mode. For instance with the current footswitch mode set to MACRo and then running a macro containing a Preset the Preset will change the mode to IGNore because the default-preset mode is IGNore. If this occurs additional footswitch presses will be ignored.

**Examples** `CONT:AUX:FOOT:MODE MACRo` This sets the footswitch mode to MACRo causing a macro to be loaded and run with a footswitch press.  
`CONTRol:AUXiliary:FOOTswitch:MODE?` This query returns the footswitch mode setting.



---

|                           |                                    |
|---------------------------|------------------------------------|
| <b>Query Syntax</b>       | CONTrol:AUXiliary:FOOTswitch:MODE? |
| <b>Return Type</b>        | Character                          |
| <b><u>Overlapped?</u></b> | No                                 |
| <b><u>Default</u></b>     | IGNore                             |

---

## CONTrol:AUXiliary:INPut:VOLTage?

(Read-Only) Reads the ADC input voltage from pin 14 of the AUX IO connector.

|                 |                                                                                    |
|-----------------|------------------------------------------------------------------------------------|
| <b>Examples</b> | <code>CONT:AUX:INPut:VOLT?</code><br><code>control:auxiliary:input:voltage?</code> |
|-----------------|------------------------------------------------------------------------------------|

|                    |         |
|--------------------|---------|
| <b>Return Type</b> | Numeric |
|--------------------|---------|

|                           |    |
|---------------------------|----|
| <b><u>Overlapped?</u></b> | No |
|---------------------------|----|

|                       |                |
|-----------------------|----------------|
| <b><u>Default</u></b> | Not Applicable |
|-----------------------|----------------|

---

## CONTrol:AUXiliary:OUTPut[1|2]:MODE <char>

(Read-Write) This command sets the mode of the selected "Analog Out" line on the Auxiliary IO. The modes give the user the option to have the requested voltage applied immediately or not until the sweep is done. Also see the description for "Analog Out 1, 2" in the Auxiliary IO connector documentation.

### Parameters

<char> **WAIT** - While in this mode any voltage changes sent to the selected analog out will only get applied to the output between sweeps.

**NOWait** - While in this mode any voltage changes sent to the selected analog out will occur right away without waiting until the end of a sweep.

|                 |                                                                                                                                         |
|-----------------|-----------------------------------------------------------------------------------------------------------------------------------------|
| <b>Examples</b> | <code>CONT:AUX:OUTP1:MOD WAIT</code> This sets the mode so that voltages sent to "Analog Out 1" are only applied at the end of a sweep. |
|-----------------|-----------------------------------------------------------------------------------------------------------------------------------------|

|  |                                                                                          |
|--|------------------------------------------------------------------------------------------|
|  | <code>CONT:AUX:OUTP2:MOD?</code> This query returns the current mode for "Analog Out 2". |
|--|------------------------------------------------------------------------------------------|

|                     |                                 |
|---------------------|---------------------------------|
| <b>Query Syntax</b> | CONTrol:AUXiliary:OUTPut2:MODE? |
|                     | 'Reads the output mode          |

|                    |           |
|--------------------|-----------|
| <b>Return Type</b> | Character |
|--------------------|-----------|

|                           |    |
|---------------------------|----|
| <b><u>Overlapped?</u></b> | No |
|---------------------------|----|

|                       |      |
|-----------------------|------|
| <b><u>Default</u></b> | WAIT |
|-----------------------|------|

---

## CONTrol:AUXiliary:OUTPut<out>:VOLTage <num>

(Read-Write) Sets and reads voltages on the DAC/Analog Output 1 and Output 2 (pins 2 and 3) of the Auxiliary IO connector.

### Parameters

- <out> DAC output number. Choose from:  
1 - DAC Output 1 (pin 2)  
2 - DAC Output 2 (pin 3)
- <num> Output Voltage. Choose a voltage value between **-10** and **+10** volts

**Examples** `CONT:AUX:OUTP1:VOLT 5`  
`control:auxiliary:output2:voltage 5`

**Query Syntax** `CONTrol:AUXiliary:OUTPut<out>:VOLTage?`  
'Reads the output DAC voltage

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## CONTrol:AUXiliary:PASSfail:LOGic <char>

(Read-Write) Sets the logic of the PassFail line ([pin 12](#)) on the AUX IO connector. This line is connected internally to the PassFail line of the Material Handler IO (pin 33).

### Parameters

- <char> Choose from:  
**POSitive** - Causes the PassFail line to have positive logic (high = pass, low = fail).  
**NEGative** - Causes the PassFail line to have negative logic (high = fail, low = pass).

**Examples** `CONT:AUX:PASS:LOG POS`  
`control:auxiliary:passfail:logic negative`

**Query Syntax** `CONTrol:AUXiliary:PASSfail:LOGic?`

**Return Type** Character

**Overlapped?** No

**Default** POSitive

---

## CONTrol:AUXiliary:PASSfail:MODE <char>

(Read-Write) Sets and reads the default logical pass/fail state. This is the state the pass/fail line stays in until a failure occurs (if the mode is NOWait), or until an end-of-sweep condition occurs (if the modes is PASS or FAIL). The end-of-sweep condition is determined by the CONTrol:AUXiliary:PASSfail:SCOPE command.

### Parameters

<char> Choose from:  
**PASS** - the line stays in PASS state until the end-of-sweep condition occurs, at which time the pass/fail line is set, and the pass/fail strobe (line 36) is activated.  
**FAIL** - the line stays in FAIL state until the end-of-sweep condition occurs, at which time the pass/fail line is set, and the pass/fail strobe (line 36) is activated.  
**NOWait** - the pass/fail line is set, and the pass/fail strobe (line 36) is activated as soon as a failure condition occurs.

### Examples

```
CONT:AUX:PASS:MODE NOW
control:auxiliary:passfail:mode fail
```

**Query Syntax** CONTrol:AUXiliary:PASSfail:MODE?

**Return Type** Character

**Overlapped?** No

**Default** NOWait

---

## CONTrol:AUXiliary:PASSfail:SCOPE <char>

(Read-Write) Sets and reads the scope of pass/fail testing. The pass/fail line can report the status of all measurements on each channel, or all measurements on all channels. This command selects which option to use.

### Parameters

<char> Choose from:  
**Channel** - A pass/fail result is computed and written to the output pins at the end of all sweeps on a channel.  
**GLOBAL** - A pass/fail result is computed and written to the output pins at the end of all sweeps on a channel.  
If the pass/fail mode is NOWait (as set by CONTrol:AUXiliary:PASSfail:MODE), the status and strobe pins are written immediately. Otherwise the pins are written as indicated above. Regardless of the mode value, the pass/fail line is returned to its default state (as set by the MODE command) at the end of channel or group of channels.

### Examples

```
CONT:AUX:PASS:SCOP CHAN
control:auxiliary:passfail:scope sweep
```

**Query Syntax** CONTrol:AUXiliary:PASSfail:SCOPE?

**Return Type** Character

**Overlapped?** No

**Default** GLOBal

---

## **CONTrol:AUXiliary:PASSfail:POLicy <char>**

(Read-Write) Sets the policy used to determine how global pass/fail is computed.

### **Parameters**

<char> Name of the policy to use. Choose from:

**ALLTests** - Pass/Fail Status returns PASS if all tests on all measurements pass.

**ALLMeas** - Pass/Fail Status returns PASS if all measurements have associated tests, and all tests pass. FAIL is returned if even one measurement has no associated limit test.

Only those measurements which are not in HOLD mode contribute to the pass/fail result.

### **Examples**

```
CONT:AUX:PASS:POL ALLM
control:auxiliary:passfail:policy alltests
```

**Query Syntax** CONTrol:AUXiliary:PASSfail:POLicy?

**Return Type** Character

**Overlapped?** No

**Default** ALLTests

---

## **CONTrol:AUXiliary:PASSfail:STATus?**

(Read-Only) Returns the most recent pass/fail status value. Use this command as follows:

1. Set the PNA trigger scope to ALL
2. Set the PNA trigger source to MANUAL or EXTERNAL.
3. Trigger the PNA.
4. Use the \*OPC? command to determine when the sweep is complete.
5. Use the **CONT:AUX:PASS:STAT?** query to obtain the global pass/fail result.

**Return Type** Character - One of the following is returned:

**PASS** - all measurements not in HOLD mode have been swept, and all associated limit tests have passed.

**FAIL** - all measurements not in HOLD mode have been swept, and one or more limit tests failed according to the specified Pass/Fail policy.

**NONE** - status cannot be determined because measurements are in progress.

**Overlapped?** No

**Default** Not Applicable

---

## CONTrol:AUXiliary:SWEepend <char>

(Read-Write) Specifies the event that will cause the AUX IO Sweep End line (pin 11) to go to a low (false) state. The line will return to a high state after the appropriate calculations are complete. This line is connected internally to the Sweep End line of the Material Handler IO.

### Parameters

<char> Choose from:

**Sweep** - the line goes low when each sweep is complete.

**Channel** - The line goes low when all of the sweeps for each channel is complete.

**Global** - The line goes low when all the sweeps for all channels are complete.

### Examples

```
CONT:AUX:SWE SWE
control:auxiliary:sweepend channel
```

**Query Syntax** CONTrol:AUXiliary:SWEepend?

**Return Type** Character

**Overlapped?** No


**Default** SWEep

---

## Control External Test Set Commands

---

Specifies the settings to remotely control the External Test Set IO connector.

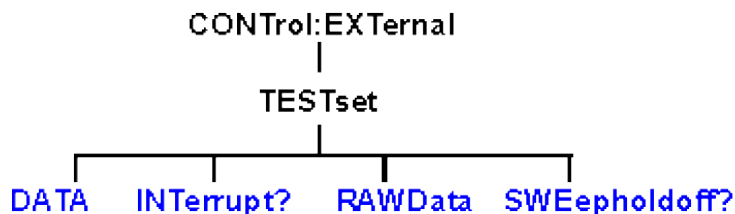

- Click on a **blue** keyword to view the command details.
  - See a [List](#) of all SCPI commands.
  - See a pinout and detailed description of the [External Test Set IO connector](#)
- 

### CONTROL:EXTernal:TESTset:DATA <addr>,<data>

(Read-Write) Reads and writes 13 bits of data to the specified address using the [AD0 through AD12](#) lines of the external test set connector. The instrument generates the appropriate timing signals (strokes the address, then the data) to control an external test set.

#### Parameters

- <addr> Decimal equivalent of the 13 bit binary address.
- <data> Decimal equivalent of the 13 bit binary data

#### Examples

```
CONT:EXT:TEST:DATA 12,3
CONTROL:external:testset:data 12,3
```



**Query Syntax** CONTROL:EXTernal:TESTset:DATA? <addr>  
'Reads the decimal equivalent of the binary data from the specified address

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

### CONTROL:EXTernal:TESTset:INTerrupt?

(Read-Only) Reads the boolean state of the Interrupt In line (pin 13) on the external test set connector.

**Examples** `CONT:EXT:TEST:INT?`  
`control:external:testset:interrupt?`

**Return Type** Boolean  
False (0) - the line is being held at a TTL High.  
True (1) - the line is being held at a TTL Low.

**Overlapped?** No

**Default** Not Applicable

---

### CONTrol:EXTernal:TESTset:RAWData <data>

(Read-Write) Reads and writes 16 bits of data through the AD0 through AD12 and three timing lines of the external test set connector. Does NOT generate appropriate timing signals.

Use of this command requires detailed knowledge of all 16 bits. Refer to the Data format table.

**Note:** During a WRITE, Bit 13 must always be low. Otherwise Bit 0-12 will tristate

---

#### Parameters

<data> Decimal equivalent of the binary data.  
Format of data **WRITTEN** with RAWData:

| Pin | Bit | Signal name |
|-----|-----|-------------|
| 22  | 0   | AD0*        |
| 23  | 1   | AD1*        |
| 11  | 2   | AD2*        |
| 10  | 3   | AD3*        |
| 9   | 4   | AD4*        |
| 21  | 5   | AD5*        |
| 20  | 6   | AD6*        |
| 19  | 7   | AD7*        |
| 6   | 8   | AD8*        |
| 5   | 9   | AD9*        |
| 4   | 10  | AD10*       |
| 17  | 11  | AD11*       |

|    |    |       |
|----|----|-------|
| 3  | 12 | AD12* |
| 25 | 13 | RLW   |
| 24 | 14 | LDS   |
| 8  | 15 | LAS   |

\* This Output will float if RLW (bit-13) is set high

**Examples**

```
CONT:EXT:TEST:RAWD 8001
CONTrol:external:testset:rawdata 1234
```

**Query Syntax**

CONTrol:EXTernal:TESTset:RAWData?

**Return Format**

Format of data **READ** with RAWData?

| Pin | Bit | Signal name                        |
|-----|-----|------------------------------------|
| 22  | 0   | AD0*                               |
| 23  | 1   | AD1*                               |
| 11  | 2   | AD2*                               |
| 10  | 3   | AD3*                               |
| 9   | 4   | AD4*                               |
| 21  | 5   | AD5*                               |
| 20  | 6   | AD6*                               |
| 19  | 7   | AD7*                               |
| 6   | 8   | AD8*                               |
| 5   | 9   | AD9*                               |
| 4   | 10  | AD10*                              |
| 17  | 11  | AD11*                              |
| 3   | 12  | AD12*                              |
| 2   | 13  | Sweep Holdoff In                   |
| 13  | 14  | Interrupt In (inverted internally) |
| na  | 15  | Always Zero, grounded internally   |



\*These lines are dependent on the state of RLW (pin25).  
Writing a 0(low) to RLW will set lines AD0-AD12 to write mode.  
Writing a 1(high) to RLW will set lines AD0-AD12 to read mode.

|                    |                |
|--------------------|----------------|
| <b>Return Type</b> | Numeric        |
| <b>Overlapped?</b> | No             |
| <b>Default</b>     | Not Applicable |

---

### **CONTRol:EXTernal:TESTset:SWEepholdoff?**

(Read-Only) Reads the Sweep Holdoff line (pin 2) on the external test set connector.

|                 |                                                                            |
|-----------------|----------------------------------------------------------------------------|
| <b>Examples</b> | <code>CONT:EXT:TEST:SWE?<br/>control:external:testset:sweepholdoff?</code> |
|-----------------|----------------------------------------------------------------------------|

|                    |                                                |
|--------------------|------------------------------------------------|
| <b>Return Type</b> | Boolean                                        |
|                    | <b>TRUE (1)</b> - the pin is set to a TTL High |
|                    | <b>FALSE (0)</b> - the pin is set to TTL Low   |

|                           |    |
|---------------------------|----|
| <b><u>Overlapped?</u></b> | No |
|---------------------------|----|


|                       |                |
|-----------------------|----------------|
| <b><u>Default</u></b> | Not Applicable |
|-----------------------|----------------|

---

## Control Handler Commands

---

Specifies the settings to remotely control the Material Handler IO connector.

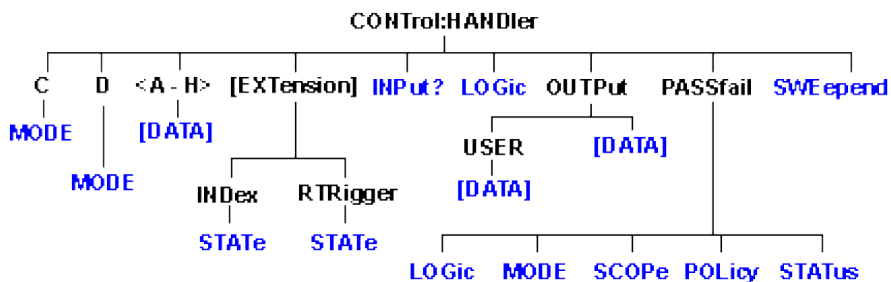

- Click on a **blue** keyword to view the command details.
  - See a [List](#) of all SCPI commands.
  - Learn about the [Material Handler IO port](#).
- 

### CONTROL:HANDler:C:MODE <char>

(Read-Write) Sets and reads the direction of data flow for Port C.

#### Parameters

<char> Direction of flow. Choose from:  
**INPut** - Port C is used to input data  
**OUTPut** - Port C is used to output data

**Examples** `CONT:HAND:C:MODE INP`  
`control:handler:c:mode output`



**Query Syntax** `CONTROL:HANDler:C:MODE?`

**Return Type** Character

**Overlapped?** No

**Default** INPut

---

### CONTROL:HANDler:D:MODE <char>

(Read-Write) Sets and reads the direction of data flow for Port D.

**Parameters**

<char> Direction of flow. Choose from:  
**INPut** - Port D is used to input data  
**OUTPut** - Port D is used to output data

**Examples** `CONT:HAND:D:MODE INP`  
`control:handler:d:mode output`

**Query Syntax** `CONTrol:HANDler:D:MODE?`

**Return Type** Character

**Overlapped?** No

**Default** Input

**CONTrol:HANDler:<port>[:DATA] <num>**

(Read-Write) Writes and reads data on the specified port.

**Parameters**

<port> Port identifier to set bits for. Choose from:  
**A,B,C,D,E,F,G,H**

<num> The number of the data bits to set. Refer to the following table for the maximum number for each port. The minimum number for each port is 0.

| Port | Max allowable <num> | MSB.....LSB<br>23.....0 |            |
|------|---------------------|-------------------------|------------|
| A    | 255                 | A7...A0                 | Write-only |
| B    | 255                 | B7...B0                 | Write-only |
| C    | 15                  | C3...C0                 | Read-Write |
| D    | 15                  | D3...D0                 | Read-Write |
| E    | 255                 | D3...D0 + C3...C0       | Read-Write |

|   |          |                                       |            |
|---|----------|---------------------------------------|------------|
| F | 65535    | B7...B0 + A7...A0                     | Write-only |
| G | 1048575  | C3...C0 + B7...B0 + A7...A0           | Write-only |
| H | 16777215 | D3...D0 + C3...C0 + B7...B0 + A7...A0 | Write-only |

---

**Note:** When writing to port G, port C must be set to output mode  
When writing to port H, both port C and port D must be set to output mode. Use CONT:HAND:C:MODE OUTP and CONT:HAND:D:MODE OUTP

---

**Examples** `CONT:HAND:A 254`  
`control:handler:c:data 12`

**Query Syntax** `CONTrol:HANDler:<port>:DATA?`

**Return Type** Numeric

**Overlapped?** No

**Default** Not Applicable

---

## **CONTrol:HANDler[:EXTension]:INDex:STATe <bool>**

(Read-Write) Determines the control of Material Handler connector Pin 20.

### **Parameters**

<char> Choose from:  
ON (1) - Pin 20 is controlled by the Index signal  
OFF (0) - Pin 20 is controlled by Output Port B6

**Examples** `CONT:HAND:IND:STAT 1`  
`control:handler:extension:index:state off`

**Query Syntax** `CONTrol:HANDler[:EXTension]:INDex:STATe?`

**Return Type** Boolean

**Overlapped?** No

**Default** OFF

---

## **CONTrol:HANDler[:EXTension]:RTRigger:STATe <bool>**

(Read-Write) Determines the control of Material Handler connector Pin 21.

**Parameters**

<char> Choose from:  
ON (1) - Pin 21 is controlled by the Ready for Trigger signal  
OFF (0) - Pin 21 is controlled by Output Port B7

**Examples** `CONT:HAND:RTR:STAT 1`  
`control:handler:extension:rtrigger:state off`

**Query Syntax** `CONTROL:HANDler[:EXTension]:RTRigger:STATE?`

**Return Type** Boolean

**Overlapped?** No

**Default** OFF

---

**CONTROL:HANDler:INPut?**

(Read-Only) Reads a hardware latch that captures high to low transitions on Input1 of the Material Handler IO. Reading the latch causes it to reset and is ready for the next transition. The hardware latch is only capable of capturing one transition per query. Additional transitions are ignored until after the next query.

Momentarily driving Input1 high, then low, will cause a transition to be detected and latched.

**Examples** `CONT:HAND:INP?`  
`control:handler:input?`

**Return Type** Integer - Returns a value of zero or one.  
**0** - A high to low transition occurred at Input1 since the last time it was queried.  
**1** - No high to low transition occurred. After the query the latch is reset and is ready for the next input. If no low to high transitions occur additional queries will return zero.

**Overlapped?** No

**Default** Not Applicable

---

**CONTROL:HANDler:LOGic <char>**

(Read-Write) Sets the logic of the Data ports A-H on the Handler connector. Some of these lines are connected internally to the AuxIO.

### Parameters

<char> Choose from:

**POSitive**- Causes the Port lines to have positive logic (high = 1, low = 0).

**NEGative**- Causes the Port lines to have negative logic (high = 0, low = 1).

For ports that are in output (write) mode, a change in logic causes the output lines to change state immediately. For example, Low levels change immediately to High levels.

For ports that are in input (read) mode (C,D,E only), a change in logic will be reflected when data is read from that port. For example, if a line read 0, the next read after a logic change will read 1.

### Examples

```
CONT:HAND:LOG POS
control:handler:logic negative
```

**Query Syntax** CONTrol:HANDler:LOGic?

**Return Type** Character

**Overlapped?** No

**Default** NEGative

---

## CONTrol:HANDler:OUTPut<port>[:DATA] <num>

(Read-Write) Sets or reads the specified output line.

Type 1 and Type 2 configurations: Returns the last value written to the selected output pin.

Type 3 configuration: Returns the current state of the selected output pin. If an Input1 trigger occurs, the state may not be the same value as was written.

### Parameters

<port> Output port. Choose from:

**1** - output 1 (default)

**2** - output 2

<num> **0** - Low

**1** - High

### Examples

```
CONT:HAND:OUTPut1 1
control:handler:output2:data 0
```

**Query Syntax** CONTrol:HANDler:OUTPut<num>:DATA?

**Return Type** Boolean

**Overlapped?** No

**Default** 0 - Low

---

## **CONTRol:HANDler:OUTPut<port>:USER[:DATA] <num>**

(Read-Write) Sets or reads the specified USER output line.

Type 1 and Type2 configurations: Returns the last value written to the selected output pin.

Type3 configuration: Returns the current state of the selected output pin. If an Input1 trigger occurs, the state may not be the same value as was written.

Learn about User Output.

### **Parameters**

<port> USER Output port. Choose from:  
1 - User output 1(default)  
2 - User output port.

<num> **0 - Low**  
**1 - High**

### **Examples**

```
CONT:HAND:OUTPut1:USER 1
control:handler:output2:user:data 0
```

**Query Syntax** CONTRol:HANDler:OUTPut<num>:USER:DATA?

**Return Type** Boolean

**Overlapped?** No

**Default** 0 - Low

---

## **CONTRol:HANDler:PASSfail:LOGic <char>**

(Read-Write) Sets the logic of the PassFail line of the Material Handler IO (pin 33). This line is connected internally to the PassFail line (pin 12) on the AUX IO connector.

**Parameters**

<char> Choose from:  
**POSitive**- Causes the PassFail line to have positive logic (high = pass, low = fail).  
**NEGative**- Causes the PassFail line to have negative logic (high = fail, low = pass).

**Examples**

```
CONT:HAND:PASS:LOG POS
control:handler:passfail:logic negative
```

**Query Syntax** CONTrol:HANDler:PASSfail:LOGic?

**Return Type** Character

**Overlapped?** No

**Default** POSitive

---

**CONTrol:HANDler:PASSfail:MODE <char>**

(Read-Write) Sets and reads the default logical pass/fail state. This is the state the pass/fail line stays in until a failure occurs (if the mode is NOWait), or until an end-of-sweep condition occurs (if the mode is PASS or FAIL). The end-of-sweep condition is determined by the CONTrol:HANDler:PASSfail:SCOPE command.

**Parameters**

<char> Choose from:  
**PASS**- the line stays in PASS state until the end-of-sweep condition occurs, at which time the pass/fail line is set, and the pass/fail strobe (line 36) is activated.  
**FAIL**- the line stays in FAIL state until the end-of-sweep condition occurs, at which time the pass/fail line is set, and the pass/fail strobe (line 36) is activated.  
**NOWait**- the pass/fail line is set, and the pass/fail strobe (line 36) is activated as soon as a failure condition occurs.

**Examples**

```
CONT:HAND:PASS:MODE NOW
control:handler:passfail:mode fail
```

**Query Syntax** CONTrol:HANDler:PASSfail:MODE?

**Return Type** Character

**Overlapped?** No

**Default** NOWait

---

**CONTrol:HANDler:PASSfail:SCOPE <char>**



(Read-Write) Sets and reads the scope of pass/fail testing. The pass/fail line on the material handler port can report the status of all measurements on each channel, or all measurements on all channels. This command selects which option to use.

### Parameters

<char> Choose from:

**CHANnel** - A pass/fail result is computed and written to the output pins at the end of all sweeps on a channel.

**GLOBal** - A pass/fail result is computed and written to the output pins at the end of all sweeps on a channel.

If the pass/fail mode is NOWait (as set by CONTrol:HANDler:PASSfail:MODE), the status and strobe pins are written immediately. Otherwise the pins are written as indicated above. Regardless of the mode value, the pass/fail line is returned to its default state (as set by the MODE command) at the end of channel or group of channels.

### Examples

```
CONT:HAND:PASS:SCOP CHAN
control:handler:passfail:scope sweep
```

**Query Syntax** CONTrol:HANDler:PASSfail:SCOPE?

**Return Type** Character

**Overlapped?** No

**Default** GLOBal

---

## CONTrol:HANDler:PASSfail:POLicy <char>

(Read-Write) Sets the policy used to determine how global pass/fail is computed.

### Parameters

<char> Name of the policy to use. Choose from:

**ALLTests** - Pass/Fail Status returns PASS if all tests on all measurements pass.

**ALLMeas** - Pass/Fail Status returns PASS if all measurements have associated tests, and all tests pass. FAIL is returned if even one measurement has no associated limit test.

Only those measurements which are not in HOLD mode contribute to the pass/fail result.

### Examples

```
CONT:HAND:PASS:POL
control:handler:passfail:policy
```

**Query Syntax** CONTrol:HANDler:PASSfail:POLicy?

**Return Type** Character

**Overlapped?** No

**Default** ALLTests

---

## CONTrol:HANDler:PASSfail:STATus?

(Read-Only) Returns the most recent pass/fail status value. Use this command as follows:

1. Set the PNA trigger scope to GLOBAL
2. Set the PNA trigger source to MANUAL or EXTERNAL.
3. Configure and enable Limit Testing
4. Trigger the PNA.
5. Use the \*OPC? command to determine when the sweep is complete.
6. Use the CONT:HAND:PASS:STAT? query to obtain the global pass/fail result.

**Return Type** Character - One of the following is returned:

**PASS** - all measurements not in HOLD mode have been swept, and all associated limit tests have passed.

**FAIL** - all measurements not in HOLD mode have been swept, and one or more limit tests failed according to the specified Pass/Fail policy.

**NONE** - status cannot be determined because measurements are in progress.

**Overlapped?** No

**Default** Not Applicable

---

## CONTrol:HANDler:SWEepend <char>

(Read-Write) Specifies the event that will cause the Handler Sweep End line to strobe. The strobe is at least 10µs in duration, and is activated when all calculations for the associated measurement are complete. This line is connected internally to the Sweep End line of the AUX IO connector.

### Parameters

<char> Choose from:

**SWEep** - the line goes low when **each sweep** is complete

**CHANnel** - the line goes low when **all the sweeps for each channel** is complete.

**GLOBAL** - the line goes low when **all sweeps for all channels** are complete.

The default state of the passFail line (before a measurement occurs) and after a failure occurs is set by CONTrol:HANDler:PASSfail:MODE

### Examples

```
CONT:HAND:SWE SWE
control:handler:sweepend channel
```

**Query Syntax** CONTrol:HANDler:SWEepend?

**Return Type** Character

**Overlapped?** No

**Default** GLOBal

---

## Local Lockout (LLO) Message

---

Normally, a GPIB instrument is put in remote mode by asserting the Remote Enable (REN) GPIB line. At that time, all front panel keys (except the Local key) are locked to prevent user interaction.

Sending the LLO message over the GPIB further locks out the keyboard, mouse, and Local key during execution of your GPIB program. The syntax of the LLO message depends on the GPIB driver you are using. Consult your GPIB software users manual.

The PNA requires these two actions to occur in order:

1. Controller sends the LLO (Local Lockout) message
2. Controller asserts the REN (Remote Enable) GPIB line

The PNA will then go into remote mode with full lockout capability.

This feature is also supported using SICL over LAN.

## Status Command Keywords

---

The following keywords can be appended to the node or nodes that represent the Status register you want to control.

**:CONDition?**

**:ENABle**

**:ENABle?**

**:EVENT?**

**:MAP**

**:NTRansition**

**:PTRansition**

[Learn about Status Registers](#)

---

**:CONDition?**

Monitors the conditions as they occur REAL TIME. That is, a condition may occur, and then clear before the condition is read. Reading this register returns a 16-bit decimal weighted number.

---

**:ENABle <bit>**

Enables register bits that will monitored using the **service request (SRQ)** method. (To use the direct read method, you do not have to enable the bit.)

Default value for `STATUS:QUESTIONable:ENABle` and `STATUS:OPERation:ENABle` is 0: No bits enabled.

Default value for all other registers `:ENABle <bits>` is 32767; ALL BITS ENABLED.

Therefore it is **ONLY** necessary to send the `ENABle` keyword if you want to **DISABLE** some conditions. For example, to enable **ONLY** Trace1 (bit 2) of the `LIMIT1` register (disable all other traces) , send:

```
STATUS:QUESTIONable:LIMit1:ENABle 4
```



**:ENABle?**

Read the enable register to verify the bits that you enabled. Returns a 16 bit weighted sum of the bits that are enabled.

---

**[:EVENT]?**

Query only - This is the Default keyword for most registers. Use it to determine if a condition has occurred. These bits remain set until they are read or otherwise cleared.

---

**:MAP <bit>,<error>**

Associates a bit is the User register with an error number. For example

```
STATUS:QUESTIONable:DEFine:USER2:MAP 0,-113
```

0 is the bit that will be set

**-113** is the error

When error -113 "Undefined Header" occurs, bit 0 in the USER2 register will be set to 1.

---

**:NTRansition <bits>**

Write-Read - Negative Transition register bits set the condition to be set on the Negative going (True to False) transition. Use this register if you are only interested in a condition changing from True to False.

**:NTRansition?**

queries the register to verify that you set a negative transition.

---

**:PTRansition <bits>**

Write-Read - Positive Transition register bits set the condition to be set on the False to True transition. Use this register if you are only interested in the change of a condition from False to True.

**:PTRansition?**

Queries the register to verify that you set a positive transition.

## Create a Balanced Measurement using SCPI

---

This example program does the following:

- creates several Balanced measurements in separate windows
- generates markers
- calculates statistics
- sets limit lines and queries results
- queries a measurement to determine if we have a balanced parameter and what type it is.

---

**Note:** By their nature, balanced measurements are extremely sensitive to phase differences between the two RF paths that make up the balanced port, especially at higher frequencies. A good calibration (not performed in this example) is critical to achieving good balanced measurement results.

---

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as `Balanced.vbs`. [Learn how to setup and run the macro.](#)

---

### See Other SCPI Example Programs

---

```
Dim app
Dim scpi
' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpIStringParser
' A comment
scpi.Execute("SYST:FPRESET")
' Put in "Single" trigger mode.
scpi.Execute("SENS:SWE:GROups:COUNT 1")
scpi.Execute("SENS:SWE:MODE GROUPS")

' This example uses DUT topology Bal-Bal -
' a DUT with a balanced input and balanced output.
'
' Port mapping for our DUT:
' logical port 1 = physical ports 1 and 4
' logical port 2 = physical ports 2 and 3
' The default is:
' logical port 1 = physical ports 1 and 2
' logical port 2 = physical ports 3 and 4
'
'
' logical 1 logical 2
'
' 1 -----| |----- 2 +
' | |
' | DUT |
' | |
' 4 -----| |----- 3 -
'
scpi.Execute("CALC:FSIM:BAL:DEvice BBALanced")
scpi.Execute("CALC:FSIM:BAL:TOPology:BBAL:PPORTs 1,4,2,3")
' Set up stimulus
scpi.Execute("SENS:SWE:POINTs 801")
scpi.Execute("SENS:FREQ:START 10e6")
```

```

scpi.Execute("SENS:FREQ:STOP 1e9")
' Turn on Four windows
scpi.Execute("DISP:WIND1:STATE ON")
scpi.Execute("DISP:WIND2:STATE ON")
scpi.Execute("DISP:WIND3:STATE ON")
scpi.Execute("DISP:WIND4:STATE ON")
' Create a trace called "sdd21", and for that trace turn on the balanced
' transformation and set the balanced transformation to BBAL SDD21.
scpi.Execute("CALC:PAR:DEF ""sdd21"",S11")
scpi.Execute("CALC:PAR:SEL ""sdd21""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDD21")
' Feed the sdd21 trace to window 1, trace 1
scpi.Execute("DISP:WIND1:TRAC1:FEED ""sdd21""")
' Similarly create 3 more balanced transmission/conversion parameters
' Create Scd21
scpi.Execute("CALC:PAR:DEF ""scd21"",S11")
scpi.Execute("CALC:PAR:SEL ""scd21""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCD21")
scpi.Execute("DISP:WIND1:TRAC2:FEED ""scd21""")
' Create Sdc21
scpi.Execute("CALC:PAR:DEF ""sdc21"",S11")
scpi.Execute("CALC:PAR:SEL ""sdc21""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDC21")
scpi.Execute("DISP:WIND1:TRAC3:FEED ""sdc21""")
' Create Scc21
scpi.Execute("CALC:PAR:DEF ""scc21"",S11")
scpi.Execute("CALC:PAR:SEL ""scc21""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCC21")
scpi.Execute("DISP:WIND1:TRAC4:FEED ""scc21""")
' Now create logical port 1 reflection parameters, and place them in window 2
scpi.Execute("CALC:PAR:DEF ""sdd11"",S11")
scpi.Execute("CALC:PAR:SEL ""sdd11""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDD11")
' Feed the sdd11 trace to window 2, trace 1
scpi.Execute("DISP:WIND2:TRAC1:FEED ""sdd11""")
' Similarly create 3 more balanced reflection/conversion parameters
scpi.Execute("CALC:PAR:DEF ""scd11"",S11")
scpi.Execute("CALC:PAR:SEL ""scd11""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCD11")
scpi.Execute("DISP:WIND2:TRAC2:FEED ""scd11""")
scpi.Execute("CALC:PAR:DEF ""sdc11"",S11")
scpi.Execute("CALC:PAR:SEL ""sdc11""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDC11")
scpi.Execute("DISP:WIND2:TRAC3:FEED ""sdc11""")
scpi.Execute("CALC:PAR:DEF ""scc11"",S11")
scpi.Execute("CALC:PAR:SEL ""scc11""")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCC11")
scpi.Execute("DISP:WIND2:TRAC4:FEED ""scc11""")
' Now create reverse transmission parameters, and place them in window 3

```



```

scpi.Execute("CALC:PAR:DEF ""sdd12"",S11")
scpi.Execute("CALC:PAR:SEL ""sdd12"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDD12")
' Feed the sdd11 trace to window 3, trace 1
scpi.Execute("DISP:WIND3:TRAC1:FEED ""sdd12"")
' Similarly create 3 more balanced reverse transmission/conversion parameters
scpi.Execute("CALC:PAR:DEF ""scd12"",S11")
scpi.Execute("CALC:PAR:SEL ""scd12"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCD12")
scpi.Execute("DISP:WIND3:TRAC2:FEED ""scd12"")
scpi.Execute("CALC:PAR:DEF ""sdc12"",S11")
scpi.Execute("CALC:PAR:SEL ""sdc12"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDC12")
scpi.Execute("DISP:WIND3:TRAC3:FEED ""sdc12"")
scpi.Execute("CALC:PAR:DEF ""scc12"",S11")
scpi.Execute("CALC:PAR:SEL ""scc12"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCC12")
scpi.Execute("DISP:WIND3:TRAC4:FEED ""scc12"")
' Now create reverse reflection parameters, and place them in window 4
scpi.Execute("CALC:PAR:DEF ""sdd22"",S11")
scpi.Execute("CALC:PAR:SEL ""sdd22"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDD22")
' Feed the sdd11 trace to window 3, trace 1
scpi.Execute("DISP:WIND4:TRAC1:FEED ""sdd22"")
' Similarly create 3 more balanced reverse reflection parameters
scpi.Execute("CALC:PAR:DEF ""scd22"",S11")
scpi.Execute("CALC:PAR:SEL ""scd22"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCD22")
scpi.Execute("DISP:WIND4:TRAC2:FEED ""scd22"")
scpi.Execute("CALC:PAR:DEF ""sdc22"",S11")
scpi.Execute("CALC:PAR:SEL ""sdc22"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SDC22")
scpi.Execute("DISP:WIND4:TRAC3:FEED ""sdc22"")
scpi.Execute("CALC:PAR:DEF ""scc22"",S11")
scpi.Execute("CALC:PAR:SEL ""scc22"")
scpi.Execute("CALC:FSIM:BAL:PAR:STATE ON")
scpi.Execute("CALC:FSIM:BAL:PAR:BBAL:DEF SCC22")
scpi.Execute("DISP:WIND4:TRAC4:FEED ""scc22"")
' Show statistics for forward differential transmission
scpi.Execute("CALC:PAR:SEL ""sdd21"")
scpi.Execute("CALC:FUNC:STATISTICS:STATE ON")
' Set up test range for markers. Set up range 1 to be between 100MHz and 900MHz
scpi.Execute("CALC:FUNC:DOMAIN:USER:START 1,100e6")
scpi.Execute("CALC:FUNC:DOMAIN:USER:STOP 1,900e6")
' Set up a marker on Sdd21, find minimum differential transmission
' Set this marker to use user-range 1 (previously defined)
scpi.Execute("CALC:PAR:SEL ""sdd21"")
scpi.Execute("CALC:MARK ON")
scpi.Execute("CALC:MARK:FUNC:DOM:USER:RANGE 1")
scpi.Execute("CALC:MARK:FUNC:EXEC MIN")

```

```

' Find Maximum common mode to differential mode conversion within user-range 1.
scpi.Execute("CALC:PAR:SEL ""sdc21"")
scpi.Execute("CALC:MARK ON")
scpi.Execute("CALC:MARK:FUNC:DOM:USER:RANGE 1")
scpi.Execute("CALC:MARK:FUNC:EXEC MAX")
' Set up limit lines
' 'MIN' Limit on Sdd21 between 100MHz and 900MHz at -2dB
scpi.Execute("CALC:PAR:SEL ""sdd21"")
scpi.Execute("CALC:LIM:SEGM:TYPE LMIN")
scpi.Execute("CALC:LIM:SEGM:STIM:START 100e6")
scpi.Execute("CALC:LIM:SEGM:STIM:STOP 900e6")
scpi.Execute("CALC:LIM:SEGM:AMPL:START -2")
scpi.Execute("CALC:LIM:SEGM:AMPL:STOP -2")
scpi.Execute("CALC:LIM:DISP:STATE ON")
scpi.Execute("CALC:LIM:STATE ON")
' 'MAX' Limit on Sdc21 between 100MHz and 900MHz at -20dB
scpi.Execute("CALC:PAR:SEL ""sdc21"")
scpi.Execute("CALC:LIM:SEGM:TYPE LMAX")
scpi.Execute("CALC:LIM:SEGM:STIM:START 100e6")
scpi.Execute("CALC:LIM:SEGM:STIM:STOP 900e6")
scpi.Execute("CALC:LIM:SEGM:AMPL:START -20")
scpi.Execute("CALC:LIM:SEGM:AMPL:STOP -20")
scpi.Execute("CALC:LIM:DISP:STATE ON")
scpi.Execute("CALC:LIM:STATE ON")
' "Single" trigger to take data.
scpi.Execute("SENS:SWE:MODE GROUPS")
response = scpi.Execute("*OPC?")
' Read the limit status byte to determine pass/fail.
' If bit 1 is set (+2), then our first measurement failed (Sdd21).
' If bit 3 is set (+8), then our third measurement failed (Sdc21).
' Both measurements failing would return +10.
response = scpi.Execute("STAT:QUES:LIM1:COND?")
If response <> 0 Then
WScript.Echo "Failure of limit lines: " & response
End If

' Here we demonstrate how to determine if we have
' a balanced parameter and what type it is.
' Read back one parameter to verify its type
scpi.Execute("CALC:PAR:SEL ""sdd21"")
' Is this a balanced parameter?
isbal = scpi.Execute("CALC:FSIM:BAL:PAR?")
' Which topology/device is set?
device = scpi.Execute("CALC:FSIM:BAL:DEV?")
device = Left(device, Len(device)-1) ' strip off newline
' Which parameter are we measuring within that topology?
balparam = scpi.Execute("CALC:FSIM:BAL:PAR:" & device & ":DEF?")
balparam = Left(balparam, Len(balparam)-1) ' strip off newline
If isbal Then
WScript.Echo "Balanced Parameter: " & balparam & " in topology: " & device & "."
Else
WScript.Echo "Parameter not balanced."
End If

```

## ECALibrate using SCPI

The following program does a 1 or 2-port Electronic Calibration using an Agilent ECAL module.

**Note:** Do NOT use `SENS:CORR:COLL:SAVE`.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive. [Learn how to setup and run the macro.](#)

### See Other SCPI Example Programs

```
' ECal full 1-port or 2-port cal
Dim pna
Dim scpi
Set pna = CreateObject("AgilentPNA835x.Application")
Set scpi = pna.ScpiStringParser
' For simplicity, this example uses the preset instrument state
scpi.Execute "SYST:PRESet"
' Turn off continuous sweep
scpi.Execute "INITiate:CONTinuous OFF"
' Select the S11 measurement that was created by the instrument preset
scpi.Execute "CALCulate:PARAMeter:SElect 'CH1_S11_1'"
' Specify the Calibration Type, and Prompt for the ECal module.
' For 2-port cal, comment out these next two lines
' and uncomment the two lines below.
scpi.Execute "SENSE:CORRection:COLLect:METHOD refl3"
MsgBox "Connect ECal module to Port 1, then press enter"
'scpi.Execute "SENSE:CORRection:COLLect:METHOD SPARSOLT"
'MsgBox "Connect ECal module to Ports 1 and 2, then press enter"
' Acquire and store the calibration terms
' then it returns reply to *OPC? when finished.
' The start and stop frequencies of your sweep must not
' extend outside the minimum or maximum frequency of your
' ECal module's characterization, or an error will be generated.
response = scpi.Execute("SENSE:CORRection:COLLect:ACQuire ECAL1;*OPC?")
MsgBox "Done with calibration."
```



## Perform an Unguided Cal on a 4-Port PNA

---

This topic describes how to perform an unguided calibration on a multiport network analyzer using SCPI. The objective here is to make clear the relationship between the physical port on which a standard is being measured, the actual device in the cal kit, and the SCPI command used to acquire the device.

There are two sets of SCPI commands that acquire calibrations. One set is used for guided cal, the other for unguided. The SCPI commands that provide remote access to unguided cal are in the SENS:CORR:COLL block:

- SENS:CORR:COLL:METHod
- SENS:CORR:COLL:ACQuire
- SENS:CORR:COLL:SAVE

On a four port network analyzer, the remote programmer needs to be aware of the relationship between the physical port and the calibration kit class assignments. The example program (below) illustrates the usage by performing three unique 2 port cals, taking care to acquire the appropriate standards.

Calibration standards classes are 'categories' of standard types. To perform a 2 port calibration, the cal wizard requires the user to measure:

### **3 reflection standards on the forward port:**

- Class S11A typically an open
- Class S11B typically a short
- Class S11C typically a load

### **Likewise, 3 reflection standards are required for the reverse port:**

- Class S22A typically an open
- Class S22B typically a short
- Class S22C typically a load

### **There is also a transmission standard that is measured in both directions:**

- Class S21T typically a thru

The following illustrates the relationship between cal kit physical standards and calibration classes.

Here is a list of the physical devices in my calibration kit.

Standard #1 = "3.5 mm male short"

Standard #2 = "3.5 mm male open"

Standard #3 = "3.5 mm male broadband load"

Standard #4 = "Insertable thru standard"

Standard #5 = "3.5 mm male sliding load"

Standard #6 = "3.5 mm male lowband load"

Standard #7 = "3.5 mm female short"

Standard #8 = "female to female characterized thru adapter"

Standard #9 = "0-2 Load"

Standard #10 = "Open"

Standard #11 = "Non-insertable thru"

Standard #12 = "3.5 mm female lowband load"

Standard #13 = "3.5 mm female sliding load"

Standard #14 = "3.5 mm female broadband load"

Standard #15 = "3.5 mm female open"

When you perform a calibration remotely using SCPI, you don't specify the device number directly. Rather, you specify the class you want to measure. Each device in the calibration kit is assigned to a class. And since more than one device can be assigned to the same class, each class contains an ordered list of devices. The class assignments are user-settable using the Advanced Modify Cal Kit dialog or the SCPI command:

SENS:CORR:COLL:CKIT:ORDER<class>, <std>, <std>, <std>, <std>, <std>, <std>, <std>

The 85052B kit used in the example program had the following standard list for each class: The list was obtained by issuing the corresponding SCPI query:

SENS:CORR:COLL:CKIT:OLIST1? S11A = +2,+15,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST2? S11B = +1,+7,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST3? S11C = +6,+5,+3,+12,+13,+14,+0

SENS:CORR:COLL:CKIT:OLIST4? S21T = +4,+8,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST5? S22A = +2,+15,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST6? S22B = +1,+7,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST7? S22C = +6,+5,+3,+12,+13,+14,+0

SENS:CORR:COLL:CKIT:OLIST8? S12T = +4,+8,+0,+0,+0,+0,+0

When you perform the calibration, you acquire data by issuing the ACQUIRE command:

SENS:CORR:COLL:ACQ <class>[, <subst> ]

For example:

SENS:CORR:COLL:SFOR 1

SENS:CORR:COLL:ACQ STANA, SST2

The SFOR command tells the wizard to make the next acquisition in the forward direction. The ACQUIRE command specifies that we are measuring the 2nd device in the list for STANA. And since we are measuring SFORward, STANA refers to class #1 or S11A. The list of devices for this class are specified in the OLIST1 query above. The associations are shown in red.

Alternately, you could modify the device order for the S11A class to move device #15 into the first position (SENS:CORR:COLL:CKIT:ORDER1). When the desired device is in the first position, you needn't specify the order number in the ACQUIRE command. The default is the first device in the OLIST. This worked well for two port network analyzers where the order for S11A,B,C classes were setup for port 1 and the order for S22A,B,C was set up for port 2. With the kit setup in the proper order, you could eliminate the specification of the substandard number (SST<n>).

When performing 2 port calibrations on 4 Port Network Analyzers (e.g.: PNA Model N5230A), the wizard applies S11A,B,C standards to the lower numbered port, S22A,B,C standards to the higher numbered port. Since the two classes (S11A,B,C and S22A,B,C) are applied to multiple ports, the programmer must take into account the ports being measured and take greater care when specifying the ACQUIRE command to ensure that the correct device is being measured.

### Port to class relationship

| Ports | S11A Port | S22A Port |
|-------|-----------|-----------|
| 1,2   | 1         | 2         |
| 1,3   | 1         | 3         |
| 1,4   | 1         | 4         |
| 2,3   | 2         | 3         |
| 2,4   | 2         | 4         |
| 3,4   | 3         | 4         |

The following example program shows one method of handling two port cals on a multiport network analyzer. The connectors at the measurement plane are assumed to be (1) male, (2) female, (3) male, and (4) male. In the example, three cals are performed: 1-2 (insertable male to female), 2-3 (insertable female to male), and 3-4 (noninsertable using an characterized adapter).

```
option explicit
public scpi
public pna
' assume a 4 port PNA with the following connectors:
' the standard measured on these ports will be the opposite gender
' PORT 1 = 3.5 male
' PORT 2 = 3.5 female
' PORT 3 = 3.5 male
' PORT 4 = 3.5 male
'To perform 2 port calibrations between 1-2, 2-3, and 3-4 you need to do the
following

call main

sub main
set pna = CreateObject("AgilentPnA835x.Application")
set scpi = pna.ScpiStringParser
pna.Preset
' select a kit to use for this demonstration
' kit #1 for the N5230A is the 85052B 3.5mm kit with sliding load
scpi.execute("SENS:CORR:COLL:CKIT:SELECT 1")
PrintKitStandardInfo 1
PrintKitOlist 1

' -----
' CALIBRATE PORTS 1 and 2, insertable cal
' -----

wscript.echo
wscript.echo "Calibrating ports 1 and 2"
scpi.execute("SYST:PRES;")
scpi.execute("calc:par:sel CH1_S11_1")
scpi.execute("SENS:CORR:TST:STATE 0")
scpi.execute("SENS:CORR:COLL:METHOD SPARSOLT")
scpi.execute("SENS:CORR:SFOR 1")
```

```

MeasureFemaleStandards 1
scpi.execute("SENS:CORR:SFOR 0")
MeasureMaleStandards 2
MeasureTransmissionStandards 1,2
scpi.execute("SENS:CORR:COLL:SAVE")

' -----
' CALIBRATE PORTS 2 and 3, insertable cal
' -----

wscript.echo
wscript.echo "Calibrating ports 2 and 3"
scpi.execute("SYST:PRES;")
scpi.execute("calc:par:sel CH1_S11_1")
scpi.execute("calc:par:mod S23")
scpi.execute("SENS:CORR:TST:STATE 0")
scpi.execute("SENS:CORR:COLL:METHod SPARSOLT")
scpi.execute("SENS:CORR:SFOR 1")
MeasureMaleStandards 2
scpi.execute("SENS:CORR:SFOR 0")
MeasureFemaleStandards 3
MeasureTransmissionStandards 2,3
scpi.execute("SENS:CORR:COLL:SAVE")

' -----
' CALIBRATE PORTS 3 and 4, non-insertable cal
' -----

wscript.echo
wscript.echo "Calibrating ports 3 and 4"
scpi.execute("SYST:PRES;")
scpi.execute("calc:par:sel CH1_S11_1")
scpi.execute("calc:par:mod S43")
scpi.execute("SENS:CORR:COLL:METHod SPARSOLT")
scpi.execute("SENS:CORR:SFOR 1")
MeasureFemaleStandards 3
scpi.execute("SENS:CORR:SFOR 0")
MeasureFemaleStandards 4
MeasureAdapter 3, 4
scpi.execute("SENS:CORR:COLL:SAVE")
end sub

sub MeasureMaleStandards (portNumber)
dim portstr
portstr = formatnumber(portNumber,0)
Promptconnect1 1, 1, portNumber
scpi.execute("SENS:CORR:COLL:ACQ STAN1;*OPC?")

Promptconnect1 2, 1, portNumber
scpi.execute("SENS:CORR:COLL:ACQ STAN2;*OPC?")
Promptconnect1 3, 3, portNumber
scpi.execute("SENS:CORR:COLL:ACQ STAN3,SST3;*OPC?")
end sub

sub MeasureFemaleStandards (portNumber)
dim portstr
portstr = formatnumber(portNumber,0)
Promptconnect1 1, 2, portNumber
scpi.execute("SENS:CORR:COLL:ACQ STAN1,SST2;*OPC?")

```

```

Promptconnect1 2, 2, portNumber
scpi.execute("SENS:CORR:COLL:ACQ STAN2,SST2;*OPC?")
Promptconnect1 3, 6, portNumber
scpi.execute("SENS:CORR:COLL:ACQ STAN3,SST6;*OPC?")
end sub

sub MeasureTransmissionStandards(port1, port2)
dim p1str
dim p2str
p1str = formatnumber(port1, 0)
p2str = formatnumber(port2, 0)

Promptconnect2 4, 1, port1, port2
scpi.execute("SENS:CORR:COLL:ACQ STAN4;*OPC?")
end sub

sub MeasureAdapter(port1, port2)
dim p1str
dim p2str
p1str = formatnumber(port1, 0)
p2str = formatnumber(port2, 0)

Promptconnect2 4, 2, port1, port2
scpi.execute("SENS:CORR:COLL:ACQ STAN4,SST2;*OPC?")
end sub

' return the nth item in the comma separated list
Function GetItemNumber(list, n)
dim strVector
strVector = split(list,",",-1,1)
GetItemNumber = strVector(n-1)
end function

' remove the trailing newline from str
function chop(str)
dim tmp
tmp = str
' remove the appended newline
dim pos
pos = InStrRev(tmp,vblf)
if (pos >0) then
tmp = mid(tmp,1,pos-1)
end if
chop = tmp
end function

'return the label for the nth standard assigned to the class described by
class_index.
' if class_index = 1, class is S11A (STAN1)
' if class_index = 2, class is S11B (STAN2), etc
function GetStandardLabel(class_index, nth)
dim olist
dim stdnum
dim resp
olist = scpi.execute("SENS:CORR:COLL:CKIT:OLIST" + formatnumber(class_index,0)+"?")
stdnum = GetItemNumber(olist, nth)
scpi.execute("SENS:CORR:COLL:CKIT:STAN " + formatnumber(stdnum,0))
resp = scpi.execute("SENS:CORR:COLL:CKIT:STAN:Label?")

```



```

GetStandardLabel = chop(resp)
end function

sub PromptConnect1(class_index, nth, port)
wscript.echo "CONNECT " + GetStandardLabel(class_index, nth) + " to port " +
formatnumber(port,0)
end sub

sub PromptConnect2(class_index, nth, port1, port2)
wscript.echo "CONNECT " + GetStandardLabel(class_index, nth) + " between ports " +
formatnumber(port1,0) + " and " + formatnumber(port2,0)
end sub

' Print the order of standards per class for this kit
sub PrintKitOlist(kit)
dim i
dim cmd
dim resp
wscript.echo
dim olistcmd
olistcmd = "SENS:CORR:COLL:CKIT:OLIST"
' list the sub standards for each of the following classes
' S11A, S11B, S11C, FWD TRANS, FWD ISOL, S22A, S22B, S22C, REV TRANS, REV ISOL
for i = 1 to 8
cmd = olistcmd + formatNumber(i,0) + "?"
resp = scpi.execute(cmd)
wscript.echo cmd + "= " + chop(resp)
next
end sub

sub PrintKitStandardInfo(kit)
wscript.echo scpi.execute("SENS:CORR:COLL:CKIT:NAME?")
dim i
for i = 1 to 30
dim slabel
dim snum
snum = formatNumber(i,0)
scpi.execute("SENS:CORR:COLL:CKIT:STAN " + snum)
slabel=scpi.execute("SENS:CORR:COLL:CKIT:STAN:LABel?")
wscript.echo "Standard #"+snum+ " = " + chop(slabel)
next
end sub

```

The output from this program is as follows:

Microsoft (R) Windows Script Host Version 5.6

Copyright (C) Microsoft Corporation 1996-2001. All rights reserved.

"85052B 3.5 mm with sliding load"

Standard #1 = "3.5 mm male short"

Standard #2 = "3.5 mm male open"

Standard #3 = "3.5 mm male broadband load"

Standard #4 = "Insertable thru standard"

Standard #5 = "3.5 mm male sliding load"

Standard #6 = "3.5 mm male lowband load"

Standard #7 = "3.5 mm female short"

Standard #8 = "female to female characterized thru adapter"

Standard #9 = "0-2 Load"

Standard #10 = "Open"

Standard #11 = "Non-insertable thru"

Standard #12 = "3.5 mm female lowband load"

Standard #13 = "3.5 mm female sliding load"

Standard #14 = "3.5 mm female broadband load"

Standard #15 = "3.5 mm female open"

Standard #16 = "Open"

Standard #17 = "Open"

Standard #18 = "Open"

Standard #19 = "Open"

Standard #20 = "Open"

Standard #21 = "Open"

Standard #22 = "Open"

Standard #23 = "Open"

Standard #24 = "Open"

Standard #25 = "Open"

Standard #26 = "Open"

Standard #27 = "Open"

Standard #28 = "Open"

Standard #29 = "Open"

Standard #30 = "Open"

SENS:CORR:COLL:CKIT:OLIST1?= +2,+15,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST2?= +1,+7,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST3?= +6,+5,+3,+12,+13,+14,+0

SENS:CORR:COLL:CKIT:OLIST4?= +4,+8,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST5?= +2,+15,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST6?= +1,+7,+0,+0,+0,+0,+0

SENS:CORR:COLL:CKIT:OLIST7?= +6,+5,+3,+12,+13,+14,+0

SENS:CORR:COLL:CKIT:OLIST8?= +4,+8,+0,+0,+0,+0,+0

Calibrating ports 1 and 2

CONNECT "3.5 mm female open" to port 1

CONNECT "3.5 mm female short" to port 1

CONNECT "3.5 mm female broadband load" to port 1

CONNECT "3.5 mm male open" to port 2

CONNECT "3.5 mm male short" to port 2

CONNECT "3.5 mm male broadband load" to port 2  
CONNECT "Insertable thru standard" between ports 1 and 2  
Calibrating ports 2 and 3  
CONNECT "3.5 mm male open" to port 2  
CONNECT "3.5 mm male short" to port 2  
CONNECT "3.5 mm male broadband load" to port 2  
CONNECT "3.5 mm female open" to port 3  
CONNECT "3.5 mm female short" to port 3  
CONNECT "3.5 mm female broadband load" to port 3  
CONNECT "Insertable thru standard" between ports 2 and 3  
Calibrating ports 3 and 4  
CONNECT "3.5 mm female open" to port 3  
CONNECT "3.5 mm female short" to port 3  
CONNECT "3.5 mm female broadband load" to port 3  
CONNECT "3.5 mm female open" to port 4  
CONNECT "3.5 mm female short" to port 4  
CONNECT "3.5 mm female broadband load" to port 4  
CONNECT "female to female characterized thru adapter" between ports 3 and 4

## Perform Global Delta Match Cal

---

The following program performs a [Global Delta Match Calibration](#). This is required when performing an Unknown Thru Cal or TRL Cal on PNAs without a reference receiver for each test port. [See example of Unknown Thru or TRL Cal](#).

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Delta.vbs. [Learn how to setup and run the macro](#).

```
Sub PerformGlobalDeltaMatchCal()
Set pna = CreateObject("AgilentPNA835x.Application")
Set scpi = pna.ScpiStringParser

' Initiate a Global Delta Match calibration, choosing connector and cal kit
scpi.Parse "SENS:CORR:COLL:GUID:DMAT 'APC 3.5 female', '85033D/E'"

' Query the number of calibration steps
retStr = scpi.Parse("SENS:CORR:COLL:GUID:STEP?")
numSteps = CInt(retStr)

' Measure the cal standards
For i = 1 To numSteps
 prompt = scpi.Parse("SENS:CORR:COLL:GUID:DESC? " & CStr(i))
 retVal = MsgBox(prompt, vbOKCancel)
 If retVal = vbCancel Then Exit Sub
 retStr = scpi.Parse("SENS:CORR:COLL:GUID:ACQ STAN" & CStr(i) & ";*OPC?")
Next

' Compute the error coefficients and save the cal to Global Delta Match CalSet
scpi.Parse "SENS:CORR:COLL:GUID:SAVE"
MsgBox "Cal is done!"
End Sub
```

## Perform a Guided Calibration using SCPI

---

This VBScript program performs a Guided Calibration using ECal or Mechanical standards. This example includes optional ECal orientation features.

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Guided.vbs. [Learn how to setup and run the macro.](#)

```
' Performing a Guided 2-port cal (Ports 1 and 2)
TwoPortGuidedCal
Sub TwoPortGuidedCal
Dim app
Dim scpi
Dim connList
Dim selectedConn
Dim kitList
Dim selectedKit
Dim message

' Create / Get the PNA application.
Set app = CreateObject("AgilentPNA835x.Application")
Set scpi = app.ScpiStringParser

' Query the list of connectors that the PNA system recognizes
connList = scpi.Execute("sens:corr:coll:guid:conn:cat?")

' Format the list with linefeed characters in place of the commas
connList = FormatList(connList)

message = "Enter your DUT connector for Port 1. Choose from this list:"
message = message & Chr(10) & Chr(10) & connList

' Select the connector for Port 1
selectedConn = InputBox(message)
If selectedConn = "" Then Exit Sub
scpi.Execute "sens:corr:coll:guid:conn:port1 '" & selectedConn & "'"

message = "Enter your DUT connector for Port 2. Again, choose from this list:"
message = message & Chr(10) & Chr(10) & connList

' Select the connector for Port 2
selectedConn = InputBox(message)
If selectedConn = "" Then Exit Sub
scpi.Execute "sens:corr:coll:guid:conn:port2 '" & selectedConn & "'"

' Note: If your PNA has more than 2 ports, then uncomment
' one or both of these next two lines.
'scpi.Execute "sens:corr:coll:guid:conn:port3 ""Not used"" "
'scpi.Execute "sens:corr:coll:guid:conn:port4 ""Not used"" "

' Query the list of acceptable cal kits and
' ECal module characterizations for Port 1.
kitList = scpi.Execute("sens:corr:coll:guid:ckit:port1:cat?")
```

```

' Format the list with linefeed
' characters in place of the commas
kitList = FormatList(kitList)

message = "Enter your cal kit or ECal module characterization for Port 1. "
message = message & "Choose from this list:"
message = message & Chr(10) & Chr(10) & kitList

' Select the Cal Kit or ECal module
' characterization to use for Port 1.
selectedKit = InputBox(message)
If selectedKit = "" Then Exit Sub
scpi.Execute "sens:corr:coll:guid:ckit:port1 '" & selectedKit & "'

' Query the list of acceptable cal kits
' and ECal module characterizations for Port 2.
kitList = scpi.Execute("sens:corr:coll:guid:ckit:port2:cat?")
' Format the list with linefeed characters in place of the commas
kitList = FormatList(kitList)

message = "Enter your cal kit or ECal module characterization for Port 2. "
message = message & "Choose from this list:"
message = message & Chr(10) & Chr(10) & kitList

' Select the Cal Kit or ECal module
' characterization to use for Port 2.
selectedKit = InputBox(message)
If selectedKit = "" Then Exit Sub
scpi.Execute "sens:corr:coll:guid:ckit:port2 '" & selectedKit & "'

' This next block of commented code
' shows optional functions when using ECal.
' Send these "sens:corr:pref" commands prior to the
' "sens:corr:coll:guid:init" command.

' Read ECAL information from ECal module #1 on the USB bus
' about the Agilent factory characterization data

'module1Info = scpi.Execute("sens:corr:coll:ckit:inf? ECAL1,CHAR0")
'MsgBox "Description of ECal Module #1:" & Chr(10) & Chr(10) & module1Info

' The following command enables auto orientation of
' the ECal module (The PNA senses which port of the
' module is connected to which port of the PNA).

'scpi.Execute "sens:corr:pref:ecal:ori ON"

' However, if you are measuring at very low power levels where
' the PNA may fail to sense the module's orientation, then turn auto
' orientation OFF and specify how the module is connected.
' "A1,B2" indicates Port A of the module is connected
' to PNA Port 1 and Port B is connected to PNA Port 2).
'scpi.Execute "sens:corr:pref:ecal:ori OFF"
'scpi.Execute "sens:corr:pref:ecal:pmap ECAL1,'A1,B2'"
' End of optional ECal setup

```

```

' Select the thru method of "Default". This instructs the PNA to
' determine which thru standard measurement technique to use
' based upon the selected connectors and
' calibration kit(s) and the PNA model number.
scpi.Execute "sens:corr:coll:guid:meth default"

' Initiate the calibration and query the number of steps
scpi.Execute "sens:corr:coll:guid:init"
numSteps = scpi.Execute("sens:corr:coll:guid:steps?")
MsgBox "Number of steps is " + CStr(numSteps)

' Measure the standards
For i = 1 To numSteps
step = "Step " + CStr(i) + " of " + CStr(numSteps)
strPrompt = scpi.Execute("sens:corr:coll:guid:desc? " + CStr(i))
MsgBox strPrompt, vbOKOnly, step
scpi.Execute "sens:corr:coll:guid:acq STAN" + CStr(i)
Next

' Conclude the calibration
scpi.Execute "sens:corr:coll:guid:save"
MsgBox "Cal is done!"

End Sub

Function FormatList(list)
Dim tokens
' Strip the leading and trailing quotation
' marks from the list string
list = Mid(list, 2, Len(list) - 3)
' Tokenize the comma-delimited list string
' into an array of the individual substrings
tokens = Split(list, ",")
' Rebuild the list string, placing linefeed
' characters where the commas were,
' using Trim to remove leading and trailing spaces.
list = ""
For i = 0 To UBound(tokens)
tokens(i) = Trim(tokens(i))
list = list & tokens(i) & Chr(9)
If i < UBound(tokens) Then
i = i + 1
tokens(i) = Trim(tokens(i))
list = list & tokens(i) & Chr(10)
End If
Next
FormatList = list
End Function

```

## Perform Guided TRL Calibration

---

This VBScript file performs a 2-Port Guided TRL calibration on **2-port PNA analyzers**. ([See an example of TRL cal on a 4-port PNA.](#)) This program does the following:

- Clear old measurements from the PNA
- Create a new S22 measurement
- Set an instrument state
- Select the connectors and cal kit
- Initiate a Guided calibration
- Display a prompt as each new standard must be connected
- Save the calibration to a newly created cal set.

---

**Note:** This program runs without error on all [PNA code revisions](#) EXCEPT 4.83 (Shipped in Jan 2005):

---

The SCPI commands in this example are sent over a COM interface using the [SCPIStringParser](#) object. You do NOT need a GPIB connection to run this example.

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as TRL.vbs. [Learn how to setup and run the macro.](#)

```
Dim App
Set App = CreateObject("AgilentPNA835x.Application")
App.Preset
Dim Meas
Dim step
Dim txtVa
Dim txtSteplofN
Dim Parser
Dim prompt
Dim txtDat
Dim Chan

Rem Clear old measurements
App.Reset

Rem Create a new Measurement
Set Parser = App.SCPIStringParser
Parser.Parse "DISPlay:WINDow1:STATE ON"
Parser.Parse "CALCulate:PARAMeter:DEFine 'MyMeas',S12"
Parser.Parse "DISPlay:WINDow1:TRACe1:FEED 'MyMeas'"

Rem Initialize state
Set Chan = App.ActiveChannel
Chan.StartFrequency = 20.0e9
Chan.StopFrequency = 22.0e9
Chan.IFBandwidth = 1000
step = 4

Rem Begin a guided calibrations
```



```

Parser.Parse "SENS:CORR:COLL:GUID:CONN:PORT1 'APC 3.5 male'"
Parser.Parse "SENS:CORR:COLL:GUID:CONN:PORT2 'APC 3.5 female'"
Parser.Parse "SENS:CORR:COLL:GUID:CKIT:PORT1 '85052C'"
Parser.Parse "SENS:CORR:COLL:GUID:CKIT:PORT2 '85052C'"

Rem Select TRL cal method
Parser.Parse "SENS:CORR:COLL:GUID:METH TRL"
txtDat = Parser.Parse("SENS:CORR:COLL:GUID:METH?")
MsgBox("Method " + txtDat)
Parser.Parse "SENS:CORR:COLL:GUID:INIT"

Rem Query the number of steps
txtDat = Parser.Parse("SENS:CORR:COLL:GUID:STEP?")

Rem Display the number of steps
MsgBox("Number of steps is " + txtDat)

Rem Set the loop counter limit
step = txtDat

Rem Measure the standards
For i = 1 To step
If i= 1 Then
prompt = Parser.Parse("sens:corr:coll:guid:desc? 1")
MsgBox(prompt)
Parser.Parse ("sens:corr:coll:guid:acq STAN1")
ElseIf i = 2 then
prompt = Parser.Parse("sens:corr:coll:guid:desc? 2")
MsgBox(prompt)
Parser.Parse ("sens:corr:coll:guid:acq STAN2")
ElseIf i = 3 then
prompt = Parser.Parse("sens:corr:coll:guid:desc? 3")
MsgBox(prompt)
Parser.Parse ("sens:corr:coll:guid:acq STAN3")
ElseIf i = 4 then
prompt = Parser.Parse("sens:corr:coll:guid:desc? 4")
MsgBox(prompt)
Parser.Parse ("sens:corr:coll:guid:acq STAN4")
End If
Next

Rem All standards have been measured. Save the result
Parser.Parse "SENS:CORR:COLL:GUID:SAVE"
MsgBox("The TRL calibration has been completed")

```

## Perform Unknown Thru or TRL Cal

---

The following program performs either a 2-port SOLT Unknown Thru Cal or a 2-port TRL Cal. The 85052C Cal Kit used in this program contains both types of standards. This program can be run on 2-port or 4-port PNAs. When run on a 4-port PNA, which does not have a reference receiver per port, a [Delta Match Cal](#) is required. See [example of Delta Match Cal](#).

This VBScript (\*.vbs) program can be run as a macro in the PNA. To do this, copy the following code into a text editor file such as Notepad and save it on the PNA hard drive as Unknown.vbs. [Learn how to setup and run the macro](#).

```
Sub PerformUnknownThruOrTRLCal()
Set pna = CreateObject("AgilentPNA835x.Application")
Set scpi = pna.ScpiStringParser

' Specify connectors for Ports 1 and 2
scpi.Parse "SENS:CORR:COLL:GUID:CONN:PORT1 'APC 3.5 female'"
scpi.Parse "SENS:CORR:COLL:GUID:CONN:PORT2 'APC 3.5 male'"

'If your PNA has 3 or 4 ports, uncomment one or both of
'these next two lines, to explicitly specify this is a 2-port cal.
'scpi.Parse "SENS:CORR:COLL:GUID:CONN:PORT3 'Not used'"
'scpi.Parse "SENS:CORR:COLL:GUID:CONN:PORT4 'Not used'"

' Specify cal kit for Ports 1 and 2
scpi.Parse "SENS:CORR:COLL:GUID:CKIT:PORT1 '85052C'"
scpi.Parse "SENS:CORR:COLL:GUID:CKIT:PORT2 '85052C'"
' Since the 85052C cal kit contains SOLT standards and also TRL
' standards, this next line determines whether the cal becomes
' unknown thru (SOLT), or TRL.
' Specify cal method
scpi.Parse "SENS:CORR:COLL:GUID:METH UNKN"

' To set up the cal as TRL, comment the previous line and uncomment this next line
'scpi.Parse "SENS:CORR:COLL:GUID:METH TRL"

' Initiate the calibration
scpi.Parse "SENS:CORR:COLL:GUID:INIT"

' Query the list of ports that need delta match
retStr = scpi.Parse("SENS:CORR:COLL:GUID:DMAT:APPL:PORT?")
portList = Split(retStr, ",")

' If portList contains just one element and it's value is 0, then that indicates
' none of the ports being calibrated require delta match data.
' Note: if each testport on the PNA has it's own reference receiver (R channel),
' then delta match is never needed, so portList will always be just 0.
lowerBound = LBound(portList)
If (UBound(portList) <> lowerBound) Or (CInt(portList(lowerBound)) <> 0) Then
' Delta match data is required for at least one port.
' For this example, we assume a Global Delta Match Cal has previously been
' performed so the Global Delta Match CalSet exists.
' The Global Delta Match CalSet is used when the APPL command is invoked
' without a specific calset ID (GUID).
scpi.Parse "SENS:CORR:COLL:GUID:DMAT:APPL"
End If
```

```
' Query the number of calibration steps
retStr = scpi.Parse("SENS:CORR:COLL:GUID:STEP?")
numSteps = CInt(retStr)

' Measure the cal standards
For i = 1 To numSteps
 prompt = scpi.Parse("SENS:CORR:COLL:GUID:DESC? " & CStr(i))
 retVal = MsgBox(prompt, vbOKCancel)
 If retVal = vbCancel Then Exit Sub
 retStr = scpi.Parse("SENS:CORR:COLL:GUID:ACQ STAN" & CStr(i) & ";*OPC?")
Next

' Compute the error coefficients and save the cal to CalSet, and turn it on
scpi.Parse "SENS:CORR:COLL:GUID:SAVE"
MsgBox "Cal is done!"
End Sub
```

## SCPI Example Programs

---

| Setup Measurements                                                                         | Environment  |
|--------------------------------------------------------------------------------------------|--------------|
| <a href="#">Catalog Measurements</a>                                                       | Visual Basic |
| <a href="#">Create a Measurement</a>                                                       | VBScript     |
| <a href="#">Channels, Windows, and Measurements using GPIB</a>                             | Visual Basic |
| <a href="#">Setup Sweep Parameters</a>                                                     | Visual Basic |
| <a href="#">Setup the Display</a>                                                          | Visual Basic |
| <a href="#">Setup a Measurement</a>                                                        | Visual C++   |
| <b>Calibrations</b> <a href="#">New</a> <a href="#">See Calibrating the PNA Using SCPI</a> |              |
| <a href="#">Guided - Comprehensive Cal</a>                                                 | VBScript     |
| <a href="#">Guided ECal</a>                                                                | VBScript     |
| <a href="#">Guided Mechanical</a>                                                          | VBScript     |
| <a href="#">Guided 1-port Mechanical Cal on Port 2</a>                                     | VBScript     |
| <a href="#">Guided TRL</a>                                                                 | VBScript     |
| <a href="#">Guided Unknown Thru or TRL Cal (apply Delta Match Cal)</a>                     | VBScript     |
| <a href="#">Global Delta Match Cal</a>                                                     | VBScript     |
| <a href="#">Unguided ECal</a>                                                              | VBScript     |
| <a href="#">Unguided 2-port Mechanical Cal</a>                                             | VBScript     |
| <a href="#">Unguided 1-port Mechanical Cal on Port 2</a>                                   | VBScript     |
| <a href="#">Perform an ECAL Confidence Check</a>                                           | Visual Basic |
| <a href="#">Perform a Source and Receiver Power Cal</a>                                    | VB/VBS       |
| <a href="#">Upload a Source Power Cal</a>                                                  | Visual Basic |
| <a href="#">Perform a Sliding Load Cal</a>                                                 | Visual Basic |
| <a href="#">Create a New Cal Kit</a>                                                       | RMB          |
| <a href="#">Modify a Calibration Kit</a>                                                   | Visual Basic |
| <b>FCA</b>                                                                                 |              |
| <a href="#">Create and Cal a VMC Measurement</a>                                           | Visual Basic |

Create and Cal an SMC Measurement Visual Basic

Create an SMC Fixed Output Measurement VBScript

### **Miscellaneous**

Getting and Putting Data Visual Basic

Getting and Putting Data (Definite Block Transfers) RMB

Transfer Data using MMEM:TRANSfer RMB

Establish a VISA Session Visual Basic

Status Reporting Visual Basic

Create a Custom Power Meter Driver Visual Basic

GPIB Pass-Through VBScript

PNA as Controller and Talker/Listener Visual Basic

See more PNA programming information and examples at: <http://na.tm.agilent.com/pna/programming/>

## Learning about COM

---

The following topics can help you learn more about controlling the PNA using COM.

[GOM versus SCPI](#)

[Configure for COM-DCOM Programming](#)

[GOM Fundamentals](#)

[Getting a Handle to an Object](#)

[GOM Collections in the PNA](#)

[PNA Automation Interfaces](#)

[GOM Data Types](#)

[Working with PNA Events](#)

[Read and Write Calibration Data using COM](#)

[C++ and the COM Interface](#)

[Using COM with .NET](#)

See more PNA programming information and examples at: <http://na.tm.agilent.com/pna/programming/>.

## Calibrating the PNA Using SCPI

---

There are several ways to calibrate the PNA using SCPI depending on your measurement needs. As from the Cal Wizard, you can perform a Guided Cal, Unguided Cal, or ECal. This topic explains the differences in these calibration choices when using SCPI commands.

### Guided Calibrations

- Use [Sens:Corr:Coll:Guided](#) commands.
- Full 1,2,3,4-port SOLT and TRL calibrations - No response calcs.
- All of the advanced calibration features (Thru method, specify DUT connectors and Cal kits for each port, port pairings).

### Unguided Calibrations

- [Sens:Correction](#) commands.
- 1-port, 2-port, Response.
- Can select 2 sets of standards.
- TRL is NOT recommended.

### ECal

From the Cal Wizard or from a SCPI program, ECal is fast, accurate, and very repeatable. Unlike from the Cal Wizard, you can use SCPI to perform ECal using either the Guided or Unguided commands. The Unguided commands are easiest to use. However, the following situations require that you use the Guided commands.

- To maximize accuracy, all ECal calibrations on the PNA perform an Unknown Thru measurement of the ECal module Thru state **IF** the [PNA model](#) being used has 1 reference receiver per port. If your PNA does NOT have 1 reference receiver per port, use Guided ECal commands and specify a Thru method.
- If your ECal module connectors do NOT match the DUT connectors, and you choose not to perform a User Characterization, use Guided ECal commands and specify the Thru method.

### ECAL Notes:

- When using either Guided or Unguided ECal commands under low power situations, use the Orientation settings. The Guided example shows the use of these commands. When using Unguided, they must appear before the Acquire command.
- The frequency range of the measurement must be within the range of the ECal module. Otherwise, the calibration will fail.
- Although we recently provided the command, you do NOT have to send the ECal module state command. The ECal algorithm switches ECal states automatically.
- All of these ECal choices are listed in the [Programming Command Search](#) function in this Help file.

See [Using ECal](#) to learn about all of the ECal features.





## Learning about GPIB

---

The following topics can help you learn more about controlling the PNA using SCPI and the GPIB.

[GPIB Fundamentals](#)

[The Rules and Syntax of SCPI Commands](#)

[Getting Data from the PNA using SCPI](#)

[Configure for VISA and SICL](#)

[Reading the PNA Status Registers](#)

[Understanding SCPI Command Synchronization](#)

See more PNA programming information and examples at: <http://na.tm.agilent.com/pna/programming/>

**AcquireCalConfidenceCheckECAL Method - OBSOLETE**

---

**Description** **Note:** This property is replaced by AcquireCalConfidenceCheckECALex Method

Transfers confidence data from the specified ECal module into the measurement's memory trace. The data is transferred to the specified S-parameter on the same channel as this Calibrator object.

The characterization within the ECal module that the confidence data will be read from is specified by the **ECALCharacterization property** on the **ICalibrator2** interface. The default value of the ECALCharacterization property is **naECALFactoryCharacterization**.

**VB Syntax** `cal.AcquireCalConfidenceCheckECAL Sparam[,ecalModule]`

---

**Variable** **(Type) - Description**

*cal* A Calibrator **(object)**

*Sparam* **(String)** S-parameter to transfer confidence data to. This parameter must be present on the same channel as the calibrator object.

*ecalModule* **(enum NAECALModule)** – Optional argument. ECal module. Choose from:

0 - naECALModule\_A (default, if unspecified)

1 - naECALModule\_B

**Return Type** None

**Default** Not applicable

---

**Examples** `Cal.AcquireCalConfidenceCheckECAL "S11", naECALModule_A`

---

**C++ Syntax** `HRESULT AcquireCalConfidenceCheckECAL( _bstr_t strParameter, enum NAECALModule ecalModule );`

**Interface** ICalibrator

## ApplyDeltaMatchFromCalSet Method

---

**Description** Specifies a Cal Set as a source of delta match correction.

If 'GUID' is not supplied then the Global Delta Match Cal Set is assumed. An error is returned if the specified Cal Set does not meet the following Delta Match criteria. The Global Delta Match Cal can ALWAYS be applied.

- Must have been performed using ECal or as a guided mechanical cal (not Unguided).
- Must have the same start freq, stop freq, and number of points as the channel being calibrated.
- Must calibrate the ports that are required by the TRL or Unknown Thru Cal as indicated by PortsNeedingDeltaMatch Property.

[Learn more about Delta match calibration.](#)

See example of a complete Delta Match calibration.

**VB Syntax** *guided*.**ApplyDeltaMatchFromCalSet** [*GUID*]

**Variable** **(Type) - Description**

*guided* GuidedCalibration (object)

*GUID* Optional Argument. GUID of the Cal Set to use. If unspecified, the Global Delta Match Cal Set is used.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `guided.ApplyDeltaMatchFromCalSet "{2B893E7A-971A-11d5-8D6C-00108334AE96}"`

**C++ Syntax** HRESULT ApplyDeltaMatchFromCalSet(BSTR calsetGUID);

**Interface** IGuidedCalibration2

## ConfigNarrowBand3 Method

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p><b>Note:</b> This method replaces <u>ConfigNarrowBand2 Method</u>. The BW argument now returns 0 if no solution is found for the specified PRF and BW. In addition, adjustments were made to the filter finder algorithm</p> <hr/> <p>This subroutine determines, then returns, the proper configuration for pulsed measurements on the PNA using the spectral nulling technique. The configuration returned needs to be sent to the PNA and any other related external equipment such as pulse generators. The routine will take a desired Pulse Repetition Frequency (PRF) and measurement IFBW and return a possibly modified PRF and IFBW for proper pulsed operation on the PNA. The routine will also return the Sample Rate, Number of Taps, and Offset that must be sent to the PNA to configure it in pulsed mode using the spectral nulling technique.</p> <p>Although the example below uses COM programming to communicate with the PNA, these commands can be replaced with <u>SCPI equivalents</u>.</p> <hr/> <p><b>Note:</b> The pulsed application may set the offset frequency (option 080) of the PNA to some value other than zero (the default value). If the stop frequency is set to the maximum of the PNA model, then an error message may appear on the PNA stating that the response frequency has exceeded the maximum allowed frequency. To fix this, set the stop frequency to a value that is at least 2 KHz less than the maximum allowed. For example, if you have a 20 GHz PNA, and the stop frequency is set to 20 GHz, and the error message appears, then set the stop frequency to 19.999998 GHz</p> <hr/> |
| <b>VB Syntax</b>   | <i>Pulsed.ConfigNarrowBand (PRF, NumTaps, BW, OffSet, SampleRate, Precision, FixedPRF, PG81110)</i>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| <i>Pulsed</i>      | <b>(interface)</b> An interface to the agilentpnapulsed.dll application interface.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <i>PRF</i>         | <p><b>(Double)</b> The Pulse Repetition Frequency.</p> <p><b>[out]</b> The pulse repetition frequency that has been optimized for use with the PNA. NOTE: This value may be different from the value requested.</p> <p><b>[in]</b> The desired pulse repetition frequency.</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <i>NumTaps</i>     | <b>(Long)</b> The number of taps to send to the PNA for pulsed operation.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <i>BW</i>          | <p><b>(Long)</b> The PNA IF Bandwidth.</p> <p><b>[out]</b> The PNA IF bandwidth that has been optimized for use with the PNA. NOTE: This value may be different from the value requested. Zero (0) is returned if no solution is found for the specified <i>PRF</i> and <i>BW</i>.</p> <p><b>[in]</b> The desired PNA IF bandwidth.</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <i>Offset</i>      | <b>(Double)</b> The offset value to send to the PNA for pulsed operation. The offset value is used to adjust the PNA for the two different possible sample rates that may be returned.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| <i>SampleRate</i>  | <b>(Double)</b> The sample rate to send to the PNA for pulsed operation.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |

*Precision* **(Double)** The precision variables sets the precision that will be used to decrement the PRF when running the configuration routines. This variable can be set to the precision required by the external pulse generators so that the configuration routine will not return a PRF that is not within the precision limits of the pulse generators.

*FixedPRF* **(Boolean)**

**1 (True)** Signals the .DLL routine to NOT adjust the PRF value; rather adjust ONLY the IF Bandwidth. This is the default setting.

**0 (False)** Adjust both the PRF and IF Bandwidth values as necessary.

*PG81110* **(Boolean)**

**1 (True)** You are using an Agilent 81110 as the pulse generator. This allows increased accuracy in adjustments for offset and PRF.

**0 (False)** Not using an Agilent 81110.

**Return Type** Not Applicable

**Default** Not Applicable

**Example** [See an example using this command.](#)

**C++ Syntax** HRESULT ConfigNarrowBand(double \*pPRF, long \*pNumTaps, long \*pBW, double \*pOffset, double \*pSampleRate, int Precision)

**Interface** AgilentPNAPulsed.Application

**ConfigNarrowBand Method OBSOLETE**

---

- Description** This method is replaced with ConfigNarrowBand2 Method which includes two new arguments.
- This subroutine determines, then returns, the proper configuration for pulsed measurements on the PNA using the spectral nulling technique. The configuration returned needs to be sent to the PNA and any other related external equipment such as pulse generators. The routine will take a desired Pulse Repetition Frequency (PRF) and measurement IFBW and return a possibly modified PRF and IFBW for proper pulsed operation on the PNA. The routine will also return the Sample Rate, Number of Taps, and Offset that must be sent to the PNA to configure it in pulsed mode using the spectral nulling technique.
- Although the example below uses COM programming to communicate with the PNA, these commands can be replaced with SCPI equivalents.
- 
- Note:** The pulsed application may set the offset frequency (option 080) of the PNA to some value other than zero (the default value). If the stop frequency is set to the maximum of the PNA model, then an error message may appear on the PNA stating that the response frequency has exceeded the maximum allowed frequency. To fix this, set the stop frequency to a value that is at least 2 KHz less than the maximum allowed. For example, if you have a 20 GHz PNA, and the stop frequency is set to 20 GHz, and the error message appears, then set the stop frequency to 19.999998 GHz
- 
- VB Syntax** *Pulsed*.**ConfigNarrowBand** (*PRF, NumTaps, BW, OffSet, SampleRate, Precision*)
- Variable** (Type) - Description
- Pulsed* **(interface)** An interface to the agilentpnapulsed.dll application interface.
- PRF* **(Double)** The Pulse Repetition Frequency.
- [out]** The pulse repetition frequency that has been optimized for use with the PNA.  
NOTE: This value may be different from the requested value.
- [in]** The desired pulse repetition frequency.
- NumTaps* **(Long)** The number of taps to send to the PNA for pulsed operation.
- BW* **(Long)** The PNA IF Bandwidth.
- [out]** The PNA IF bandwidth that has been optimized for use with the PNA. NOTE: This value may be different from the value requested.
- [in]** The desired PNA IF bandwidth.
- Offset* **(Double)** The offset value to send to the PNA for pulsed operation. The offset value is used to adjust the PNA for the two different possible sample rates that may be returned.
- SampleRate* **(Double)** The sample rate to send to the PNA for pulsed operation.
- Precision* **(Double)** The precision variables sets the precision that will be used to decrement the PRF when running the configuration routines. This variable can be set to the precision required by the external pulse generators so that the configuration routine will not return a PRF that is not within the precision limits of the pulse generators.

**Return Type** Not Applicable

**Default** Not Applicable

**Example** [See an example using this command.](#)

**C++ Syntax** HRESULT ConfigNarrowBand(double \*pPRF, long \*pNumTaps, long \*pBW, double \*pOffset, double \*pSampleRate, int Precision)

**Interface** AgilentPNAPulsed.Application

Write-only

## CreateCustomMeasurement Method OBSOLETE

---

|                    |                                                                                                                                                                                                                          |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | This command is replaced with <u>CreateCustomMeasurementEx Method</u> .<br>Creates a new custom measurement.                                                                                                             |
| <b>VB Syntax</b>   | <code>app.CreateCustomMeasurement chanNum, guid[, window]</code>                                                                                                                                                         |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                              |
| <i>app</i>         | <b>(object)</b> - An <u>Application</u> object                                                                                                                                                                           |
| <i>chanNum</i>     | <b>(long)</b> -Channel number used by the new measurement; can exist or be a new channel.                                                                                                                                |
| <i>guid</i>        | <b>(string)</b> - the GUID (Globally Unique Identifier) of the new custom measurement object. The new custom measurement must be installed and registered on the PNA. Should be in "registry format". See example below. |
| <i>window</i>      | <b>(long)</b> Optional argument. Number of the window the new custom measurement will be placed in. Choose <b>1</b> to <b>16</b> . If unspecified, the measurement is placed in the active window.                       |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                           |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                           |
| <b>Examples</b>    | <pre>app.CreateCustomMeasurement 1, "{12345678-56D3-11D5-AD50-00108334AE98}" 'Not an actual custom measurement - for example purpose only</pre>                                                                          |
| <b>C++ Syntax</b>  | HRESULT CreateCustomMeasurement (long ChannelNum, BSTR guid, long windowNumber)                                                                                                                                          |
| <b>Interface</b>   | IApplication                                                                                                                                                                                                             |



**CreateS-Parameter Method - OBSOLETE**

---

|                    |                                                                                                                                                                                                       |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This method is replaced by <a href="#">Create SParameterEX</a> method which also allows the selection of a load port                                                                     |
|                    | This method creates a new S-Parameter measurement in an existing or new window.                                                                                                                       |
| <b>VB Syntax</b>   | <code>app.CreateSParameter chan,recvr,source,[window]</code>                                                                                                                                          |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                           |
| <i>app</i>         | <u>Application</u> ( <b>object</b> )                                                                                                                                                                  |
| <i>chan</i>        | <b>(long integer)</b> - Channel number of the new measurement                                                                                                                                         |
| <i>recvr</i>       | <b>(long integer)</b> - Port number of the receiver (1 or 2)                                                                                                                                          |
| <i>source</i>      | <b>(long integer)</b> - Port number of the source (1 or 2)                                                                                                                                            |
| <i>window</i>      | <b>(long integer)</b> - Optional argument. Window number of the new measurement. Choose 1 to 4. If unspecified, the S-Parameter will be created in the Active Window.                                 |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                        |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                        |
| <b>Examples</b>    | <pre>app.CreateSParameter 1,2,1,1 'Creates a new S21 measurement in channel 1 and New window(1) app.CreateSParameter 1,2,1 'Creates a new S21 measurement in channel 1 and in the active window</pre> |
| <b>C++ Syntax</b>  | <code>HRESULT CreateSParameter(long ChannelNum, long RcvPort, long SrcPort, long windowNumber)</code>                                                                                                 |
| <b>Interface</b>   | IApplication                                                                                                                                                                                          |

**DataToDivisor Method** OBSOLETE

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This property is replaced by <a href="#">DoReceiverPowerCal Method</a> .<br><br>Stores the measurement's data to the measurement's "divisor" buffer for use by the Normalization data processing algorithm. Normalization is currently supported only on measurements of unratiod power, for purpose of receiver power calibration. If DataToDivisor is called on a ratioed measurement (such as an S-parameter), it will return an error. |
| <b>VB Syntax</b>   | <i>meas</i> .DataToDivisor                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                             |
|                    | <i>meas</i> <b>(object)</b> - A Measurement object                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>Return Type</b> | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <b>Examples</b>    | <code>meas.DataToDivisor</code>                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>C++ Syntax</b>  | HRESULT DataToDivisor();                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Interface</b>   | IMeasurement                                                                                                                                                                                                                                                                                                                                                                                                                                            |

Write-only

## DoECAL1Port Method - OBSOLETE

---

**Description** **Note:** This property is replaced by [DoECAL1PortEx Method](#).

Does a 1-Port calibration using an ECAL module. You must first have a 1-port measurement active to perform the calibration.

The characterization within the ECAL module that will be used for the calibration is specified by the [ECALCharacterization property](#) on the [ICalibrator2](#) interface. The default value of the ECALCharacterization property is [naECALFactoryCharacterization](#).

**VB Syntax** `cal.DoECAL1Port [port][,module]`

---

**Variable** **(Type) - Description**

`cal` A Calibrator (**object**)

`port` (**long integer**) Optional argument - Port number to calibrate. Choose from:  
 1 - Calibrate port 1 (default if unspecified)  
 2 - Calibrate port 2

`module` (**enum NAECALModule**) Optional argument - ECAL module. Choose from:  
 0 - naECALModule\_A - (default if unspecified)  
 1 - naECALModule\_B

**Return Type** None

**Default** Not Applicable

---

**Examples** `cal.DoECAL1Port, 2, naECALModule_B`

---

**C++ Syntax** `HRESULT DoECAL1Port(long port, tagNAECALModule ecalModule);`

**Interface** ICalibrator

**DoECAL2Port Method - OBSOLETE**


---

**Description** **Note:** This property is replaced by DoECAL2PortEx Method.

Does a 2-Port calibration using an ECAL module. You must first have a 2-port measurement active to perform the calibration.

The characterization within the ECal module that will be used for the calibration is specified by the **ECALCharacterization property** on the **ICalibrator2** interface. The default value of the ECALCharacterization property is **naECALFactoryCharacterization**.

**VB Syntax** *cal.DoECAL2Port[portA][,portB][,module]*

---

**Variable** **(Type) - Description**

*cal* A Calibrator (**object**)

*portA* (**long integer**) Optional argument - Number of the receive port to calibrate.  
Choose from:  
1 - Calibrate port 1 (default, if unspecified)  
2 - Calibrate port 2  
3 - Calibrate port 3 (if the PNA has 3 ports)

*portB* (**long integer**) Optional argument - Number of the source port to calibrate.  
Choose from:  
1 - Calibrate port 1 (default, if unspecified)  
2 - Calibrate port 2  
3 - Calibrate port 3 (if the PNA has 3 ports)

*module* (**enum NAECALModule**) – Optional argument. ECal module.  
Choose from:  
0 - naECALModule\_A (default, if unspecified)  
1 - naECALModule\_B

**Return Type** None

**Default** Not Applicable

---

**Examples** `cal.DoECAL2Port,1,2,naECALModule_B`

---

**C++ Syntax** HRESULT DoECAL2Port(long rcvport, long srcPort, tagNAECALModule ecalModule);

**Interface** ICalibrator

Write-only

## GenerateGlobalDeltaMatchSequence Method

---

**Description** Initiates a global delta match calibration.

[Learn more about Delta match calibration.](#)

See example of a complete Delta Match calibration.

**VB Syntax** *numSteps* = *guided*.**GenerateGlobalDeltaMatchSequence** *conn*,*cKit*

**Variable** **(Type) - Description**

*numSteps* **Long Integer** - Variable to store the returned number of connection steps required by the Global Delta Match Cal.

*guided* [GuidedCalibration](#) (object)

*conn* **String** Connector Type for port 1.

*cKit* **String** Cal Kit for all ports.

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `guided.GenerateGlobalDeltaMatchSequence "APC 3.5 female", "85052B"`

**C++ Syntax** HRESULT GenerateGlobalDeltaMatchSequence(BSTR port\_1\_conn, BSTR cal\_kit, long \*num\_steps);

**Interface** IGuidedCalibration2

Read-only

## GetECALModuleInfo Method - OBSOLETE

---

|                         |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
|-------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b>      | <p><b>Note:</b> This property is replaced by <a href="#">GetECALModuleInfoEx Method</a></p> <p>Returns the following information about the connected ECAL module: model number, serial number, connector type, calibration date, min and max frequency.</p> <p>The characterization within the ECAL module that this information will be read from is specified by the <b>ECALCharacterization property</b> on the <b>ICalibrator2</b> interface. The default value of the ECALCharacterization property is <b>naECALFactoryCharacterization</b>.</p> |
| <b>VB Syntax</b>        | <code>moduleInfo = cal.GetECALModuleInfo (module)</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Variable</b>         | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| <code>moduleInfo</code> | <b>(string)</b> - variable to store the module information                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <code>cal</code>        | A Calibrator <b>(object)</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <code>module</code>     | <b>(enum NAECALModule)</b> – ECAL module. Choose from:<br>0 - naECALModule_A<br>1 - naECALModule_B                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
| <b>Return Type</b>      | String                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Default</b>          | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
| <b>Examples</b>         | <pre>info = cal.GetECALModuleInfo(naECALModule_A)</pre> <p><b>Example return string:</b></p> <pre>ModelNumber: 85092-60007, SerialNumber: 01386, ConnectorType: N5FN5F, PortAConnector: Type N (50) female, PortBConnector: Type N (50) female, MinFreq: 30000, MaxFreq: 9100000000, NumberOfPoints: 250, Calibrated: July 4 2002</pre>                                                                                                                                                                                                               |
| <b>C++ Syntax</b>       | <code>HRESULT GetECALModuleInfo(tagNAECALModule ecalModule, BSTR* info);</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Interface</b>        | ICalibrator                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |

**getSourcePowerCalDataScalar Method - OBSOLETE**

**Description** Retrieves (as scalar values) requested source power calibration data, if it exists, from this channel.

**Note:** This method is replaced by [GetSourcePowerCalDataScalarEx Method](#)

**VB Syntax** `chandata.getSourcePowerCalDataScalar sourcePort, numValues, data`

**Variable** **(Type) - Description**

`chandata` **(interface)** – An ISourcePowerCalData interface pointing to a Channel (object)

`sourcePort` **(long integer)** – The source port for which calibration data is being requested.

`numValues` **(long integer)** – Number of data values.

[out] – specifies number of data values returned.

[in] – specifies number of values being requested (this must not be larger than the capacity of the data array).

`data` **(single)** – Array to store the data.

**Return Type** Single

**Default** Not Applicable

**Examples**

```
Dim numValues As Long
Dim scalarCalValues() As Single
Dim chanData As ISourcePowerCalData
Const port1 As Long = 1
numValues = app.ActiveChannel.NumberOfPoints
ReDim scalarCalValues(numValues)
Set chanData = app.ActiveChannel

chanData.getSourcePowerCalDataScalar port1, numValues,
scalarCalValues(0)

'Print the data
For i = 0 to numValues - 1
Print scalarCalValues(i)
Next I
```

**C++ Syntax** HRESULT getSourcePowerCalDataScalar(long sourcePort, long \*pNumValues, float \*pVals);

**Interface** ISourcePowerCalData

**getSourcePowerCalData Method - OBSOLETE**

---

**Description** Retrieves (as variant data type) requested source power calibration data, if it exists, from this channel.

---

**Note:** This method is replaced by [GetSourcePowerCalDataEx Method](#).

---

**Note:** This method returns a variant which is less efficient than methods available on the [ISourcePowerCalData](#) interface

---

**VB Syntax** `data = chan.getSourcePowerCalData sourcePort`

**Variable** **(Type) - Description**

`data` **(variant)** – Array to store the data.

`chan` **(object)** – A Channel object

`sourcePort` **(long integer)** – The source port for which calibration data is being requested.

**Return Type** Variant array – automatically dimensioned to the size of the data.

**Default** Not Applicable

**Examples**

```
Dim varData As Variant
Const port1 As Long = 1
varData = chan.getSourcePowerCalData port1
'Print the data
For i = 0 to chan.NumberOfPoints - 1
Print varData(i)
Next i
```

**C++ Syntax** `HRESULT getSourcePowerCalData(long sourcePort, VARIANT *pData);`

**Interface** `IChannel`



**GetStandard Method - OBSOLETE**

---

**Description** This command has been replaced with [Get StandardByString](#)

Retrieves data that was acquired for a specific cal standard. This method returns the actual measurement data - not the calculated error terms.

This method returns a variant which is less efficient than [getStandardComplex](#) on the ICalData interface.

[Learn about reading and writing Calibration data.](#)

**VB Syntax** `data = cal.getStandard(class,rcv,src)`

**Variable (Type) - Description**

`data` Variant array to store the data.

`cal` A Calibrator (**object**)

`class` (**enum NACalClass**) Standard to be measured. Choose from:

1 - naClassA

2 - naClassB

3 - naClassC

4 - naClassD

5 - naClassE

6 - naReferenceRatioLine

7 - naReferenceRatioThru

**SOLT Standards**

1 - naSOLT\_Open

2 - naSOLT\_Short

3 - naSOLT\_Load

4 - naSOLT\_Thru

5 - naSOLT\_Isolation

**TRL Standards**

1 - naTRL\_Reflection

2 - naTRL\_Line\_Reflection

3 - naTRL\_Line\_Tracking

4 - naTRL\_Thru

5 - naTRL\_Isolation

*rcv* **(long integer)** - Receiver Port

*src* **(long integer)** - Source Port

**Return Type** **(variant)** - two-dimensional array (0:1, 0:NumberOfPoints-1)

**Default** Not Applicable

**Examples**

```
Dim varStd As Variant
varStd = cal.getStandard(naSOLT_Thru,2,1)
```

**C++ Syntax** HRESULT raw\_getStandard(tagNACalClass stdclass, long ReceivePort, long SourcePort, VARIANT\* pData)

**Interface** ICalibrator

---

**putSourcePowerCalDataScalar Method - OBSOLETE**

---

|                          |                                                                                                                                                                                                     |
|--------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b>       | <u>Note: This method is replaced by <a href="#">PutSourcePowerCalDataScalarEx Method</a></u><br>Inputs source power calibration data (as scalar values) to this channel for a specific source port. |
| <b>VB Syntax</b>         | <i>chandata.putSourcePowerCalDataScalar sourcePort, numValues, data</i>                                                                                                                             |
| <b>Variable</b>          | <b>(Type) - Description</b>                                                                                                                                                                         |
| <i>chandata</i>          | <b>(interface)</b> – – An ISourcePowerCalData interface pointing to a Channel (object)                                                                                                              |
| <i>sourcePort</i>        | <b>(long integer)</b> – The source port for which calibration data is being input.                                                                                                                  |
| <i>numValues</i>         | <b>(long integer)</b> – Number of data values being input.<br><hr/> <b>Note:</b> If this does not equal the current number of points on the channel, the calibration will not be valid. <hr/>       |
| <i>data</i>              | <b>(single)</b> – Array of source power cal data being input.                                                                                                                                       |
| <b>Return Type</b>       | None                                                                                                                                                                                                |
| <b>Default</b>           | Not Applicable                                                                                                                                                                                      |
| <b>Examples</b>          | <pre>Dim chanData As ISourcePowerCalData Set chanData = app.ActiveChannel chanData.putSourcePowerCalDataScalar 1, 201, scalarCalValues(0)</pre>                                                     |
| <b><u>C++</u> Syntax</b> | HRESULT putSourcePowerCalDataScalar(long sourcePort, long numValues, float *pVals);                                                                                                                 |
| <b>Interface</b>         | ISourcePowerCalData                                                                                                                                                                                 |

**putSourcePowerCalData Method OBSOLETE**

---

**Description** Inputs source power calibration data (as variant data type) to this channel for a specific source port.

**Note:** This method is obsolete. It is replaced by PutSourcePowerCalDataEx Method

**VB Syntax** *chan.putSourcePowerCalData sourcePort, data*

**Variable (Type) - Description**

*chan* **(object)** – A Channel object

*sourcePort* **(long integer)** – The source port for which calibration data is being requested.

*data* **(variant)** – Array of source power cal data being input.

**Return Type** None

**Default** Not Applicable

**Examples** `chan.putSourcePowerCalData 1, varData`

**C++ Syntax** HRESULT putSourcePowerCalData(long sourcePort, VARIANT varData);

**Interface** IChannel

**PutStandard Method - OBSOLETE**

---

**Description** **Note:** This command is replaced by [PutStandardByString](#)

Writes variant data to the error correction buffer holding measurement data acquired for a specific standard.

[Learn about reading and writing Calibration data.](#)

**VB Syntax** `cal.putStandard class,rcv,src,data`

**Variable** **(Type) - Description**

`cal` A Calibrator (**object**)

`class` (**enum NACalClass**) Standard. Choose from:

- 1 - naClassA
- 2 - naClassB
- 3 - naClassC
- 4 - naClassD
- 5 - naClassE
- 6 - naReferenceRatioLine
- 7 - naReferenceRatioThru

**SOLT Standards**

- 1 - naSOLT\_Open
- 2 - naSOLT\_Short
- 3 - naSOLT\_Load
- 4 - naSOLT\_Thru
- 5 - naSOLT\_Isolation

**TRL Standards**

- 1 - naTRL\_Reflection
- 2 - naTRL\_Line\_Reflection
- 3 - naTRL\_Line\_Tracking
- 4 - naTRL\_Thru
- 5 - naTRL\_Isolation

`rcv` (**long**) - Receiver Port

`src` (**long**) - Source Port

*data* **(variant)** Two dimensional array (0:1, 0:points-1)

**Return Type** Not Applicable

**Default** Not Applicable

**Examples** `Dim varStd (1,200) As Variant  
cal.putStandard naSOLT_Thru, 2, 1, varStd`

**C++ Syntax** HRESULT raw\_putStandard(tagNACalClass stdclass, long ReceivePort, long SourcePort, VARIANT varData)

**Interface** ICalibrator

**SetCalInfo Method (for source power cal)**

---

**Description** Specifies the technique to be used for the source power calibration about to be performed, and the channel and source port for which it is to be performed.

**VB Syntax** *powerCalibrator*.**SetCalInfo** *calMethod, channel, sourcePort, calPower*

**Variable** **(Type) - Description**

*powerCalibrator* **(object)** - A SourcePowerCalibrator object

*calMethod* **(enum NASourcePowerCalMethod)** The method of gathering the source power correction data.

**0 – naPowerMeter** (the only method currently supported)

*channel* **(long integer)** - Number of the PNA channel (not power meter channel) on which the source power cal will be performed. If the channel doesn't already exist, it will be created.

*sourcePort* **(long integer)** - Port number on which the source power cal will be performed.

*calPower* **(double)** - Specifies the power level that is expected at the desired reference plane (input or output of DUT) following the source power cal.

**Return Type** None

**Default** Not Applicable

**Examples** `powerCalibrator.SetCalInfo naPowerMeter, 1, 1, -10`

**C++ Syntax** HRESULT SetCalInfo(tagNASourcePowerCalMethod calMethod, long channel, long sourcePort, double calPower);

**Interface** ISourcePowerCalibrator

## E5091Testsets Collection

---

### Description

There can be two testsets connected and controlled by the PNA at any time.

The item number in the testsets collection is set by the DIP switches on the testset rear-panel. The valid item numbers are 1 and 2. If the testset DIP switches are set to 1, then item number in the collection is 1, and so forth. See your E5091A documentation for more information.

If the specified testset is not connected to USB or not ON, then setting Enabled = True will return an error. All other properties can be set when the testset is not connected.

### Accessing the E5091Testsets collection

Child of the **Application** Object. Get a handle to one of the E5091Testset objects by specifying an item of the collection.

```
Dim pna
Set pna = CreateObject("AgilentPNA835x.Application")
Dim testsets As E5091Testsets
Set testsets = pna.E5091Testsets
Dim tset1 As E5091Testset
Set tset1 = testsets(1)
```

### See Also:

[E5091Testset Control COM Example](#)

[E5091 TestSet Control](#)

[Collections in the Analyzer](#)

[The PNA Object Model](#)

[E5091Testset Object](#)

| Methods | Description                                         |
|---------|-----------------------------------------------------|
| Item    | Use to get a handle to a testset in the collection. |



| Properties | Description                                                    |
|------------|----------------------------------------------------------------|
| Count      | Returns the number of items in a collection of objects.        |
| Parent     | Returns a handle to the current naNetworkAnalyzer application. |

### E5091Testsets History

| Interface      | Introduced with PNA Rev: |
|----------------|--------------------------|
| IE5091Testsets | 5.2                      |



## E5091Testset Object

---

### Description

There can be two testsets connected and controlled by the PNA at any time.

The item number in the testsets collection is set by the DIP switches on the testset rear-panel. The valid item numbers are 1 and 2. If the testset DIP switches are set to 1, then item number in the collection is 1, and so forth. See your E5091A documentation for more information.

If the specified testset is not connected to USB or not ON, then setting Enabled = True will return an error. All other properties can be set when the testset is not connected.

### Accessing the E5091Testset object

Child of the **Application** Object. Get a handle to one of the testsets by specifying an item of the collection.

```
Dim pna
Set pna = CreateObject("AgilentPNA835x.Application")
Dim testsets As E5091Testsets
Set testsets = pna.E5091Testsets
Dim tset1 As E5091Testset
Set tset1 = testsets(1)
```

### See Also:

[E5091Testset Control COM Example](#)

[E5091 TestSet Control](#)

[E5091Testsets Collection](#)

[The PNA Object Model](#)

| Methods | Description |
|---------|-------------|
|---------|-------------|

None

| Properties | Description |
|------------|-------------|
|------------|-------------|

|                               |                                                                                  |
|-------------------------------|----------------------------------------------------------------------------------|
| <a href="#">ControlLines</a>  | Sets the control lines of the specified E5091A.                                  |
| <a href="#">Enabled</a>       | Turns ON/OFF the port switching and control line output of the specified E5091A. |
| <a href="#">ID</a>            | Returns the test set ID number.                                                  |
| <a href="#">NumberOfPorts</a> | Reads the number of ports (7 or 9) that are on the specified E5091A Testset.     |
| <a href="#">OutputPort</a>    | Switches an input to one of the valid outputs on the specified E5091A.           |

### E5091Testset History

| <b>Interface</b> | <b>Introduced with PNA Rev:</b> |
|------------------|---------------------------------|
|------------------|---------------------------------|

|               |     |
|---------------|-----|
| IE5091Testset | 5.2 |
|---------------|-----|

Write/Read

## ECALCharacterization Property - OBSOLETE

---

|                    |                                                                                                                                                                                                                                                                                                                                         |
|--------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This property is replaced by <a href="#">ECALCharacterizationEx Property</a> .<br>Specifies the characterization data within an ECal module to be used for the calibration.<br>Learn more about <a href="#">ECal User Characterization</a> .                                                                               |
| <b>VB Syntax</b>   | <i>cal</i> . <b>ECALCharacterization</b> ( <i>mod</i> ) = <i>value</i>                                                                                                                                                                                                                                                                  |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                             |
| <i>cal</i>         | <a href="#">Calibrator</a> (object)                                                                                                                                                                                                                                                                                                     |
| <i>module</i>      | 1- ECal module                                                                                                                                                                                                                                                                                                                          |
| <i>value</i>       | <b>(Long)</b> – Characterization data within the ECal module to be used for ECal operations.<br>Choose from:<br><b>0</b> – Factory Characterization<br><b>1</b> – UserCharacterization1<br><b>2</b> – UserCharacterization2<br><b>3</b> – UserCharacterization3<br><b>4</b> – UserCharacterization4<br><b>5</b> – UserCharacterization5 |
| <b>Return Type</b> | Long                                                                                                                                                                                                                                                                                                                                    |
| <b>Default</b>     | <b>0</b> - Factory Characterization                                                                                                                                                                                                                                                                                                     |
| <b>Interface</b>   | ICalibrator2                                                                                                                                                                                                                                                                                                                            |

**ECALPortMap Property - OBSOLETE**

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <p><b>Note:</b> This command is replaced by <a href="#">ECALPortMapEx</a></p> <p>Specifies which ports of the ECal module are connected to which ports of the PNA for the <a href="#">DoECAL1Port</a> and <a href="#">DoECAL2Port</a> methods when the <a href="#">OrientECALModule</a> property = False.</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| <b>VB Syntax</b>   | <i>cal</i> . <b>ECALPortMap</b> = <i>value</i>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <i>cal</i>         | A Calibrator ( <b>object</b> )                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <i>value</i>       | <p><b>(string)</b></p> <p><b>(string)</b> -Format this parameter in the following manner:<br/>Aw,Bx,Cy,Dz<br/>where</p> <ul style="list-style-type: none"> <li>• A, B, C, and D are literal ports on the ECAL module</li> <li>• w,x,y, and z are substituted for PNA port numbers to which the ECAL module port is connected.</li> </ul> <p>Ports of the module which are not used are omitted from the string.<br/>For example, on a 4-port ECal module with</p> <ul style="list-style-type: none"> <li>• port A connected to PNA port 2</li> <li>• port B connected to PNA port 3</li> <li>• port C not connected</li> <li>• port D connected to PNA port 1</li> </ul> <p>the string would be: A2,B3,D1</p> <p><a href="#">DoECAL1Port</a> or <a href="#">DoECAL2Port</a> methods will fail if the port numbers passed to those methods are not in the string of this property and <a href="#">OrientECALModule</a> property = False.</p> |
| <b>Return Type</b> | String                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>Default</b>     | Not Applicable                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Examples</b>    | <pre>Dim cal As Calibrator Dim sPortMap As String Set cal = PNAapp.ActiveChannel.Calibrator cal.ECALPortMap = "a2,b1" 'Write sPortMap = cal.ECALPortMap 'Read</pre>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |

**C++ Syntax** HRESULT put\_ECALPortMap(tagNAECALModule ecalModule, BSTR strPortMap);  
HRESULT get\_ECALPortMap(tagNAECALModule ecalModule, BSTR \*strPortMap);

**Interface** ICalibrator3

## InterpolateNormalization Property **OBSOLETE**

---

**Description** **Note:** This property is replaced by `DoReceiverPowerCal` Method.

Turns ON and OFF normalization interpolation which calculates new divisor data when stimulus values change after normalization.

When this property is ON and normalization is being applied, the Normalization algorithm attempts to interpolate the divisor data whenever the stimulus parameters are changed.

When this property is OFF under the same circumstances, normalization is turned OFF.

Normalization is currently supported only on measurements of unratiod power for the purpose of performing a receiver power calibration.

**VB Syntax** `meas.InterpolateNormalization = value`

**Variable** **(Type) - Description**

`meas` **(object)** - A Measurement object

`value` **(boolean)**

0 – Turns normalization interpolation OFF

1 – Turns normalization interpolation ON

**Return Type** Boolean

**Default** 0 -OFF

**Examples** `meas.InterpolateNormalization = 1 'Write`

`normalized = meas.InterpolateNormalization 'Read`

**C++ Syntax** `HRESULT put_InterpolateNormalization(VARIANT_BOOL bState);`  
`HRESULT get_InterpolateNormalization(VARIANT_BOOL *bState);`

**Interface** IMeasurement

**IsECALModuleFound Property - OBSOLETE**

---

|                    |                                                                                                                                                                                                                                     |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This property is replaced by <a href="#">IsECALModuleFoundEx Property</a> .<br>Tests communication between the PNA and the specified ECal module.                                                                      |
| <b>VB Syntax</b>   | <code>modFound = cal.IsECALModuleFound (module)</code>                                                                                                                                                                              |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                         |
| <i>modFound</i>    | <b>(boolean)</b> - Variable to store the returned test result.<br><b>True</b> - The PNA identified the presence of the specified ECal module.<br><b>False</b> - The PNA did NOT identify the presence of the specified ECal module. |
| <i>cal</i>         | <b>(object)</b> - A Calibrator object                                                                                                                                                                                               |
| <i>module</i>      | <b>(enum NAECALModule)</b> – ECAL module. Choose from:<br>0 - naECALModule_A<br>1 - naECALModule_B                                                                                                                                  |
| <b>Return Type</b> | Boolean                                                                                                                                                                                                                             |
| <b>Default</b>     | Not applicable                                                                                                                                                                                                                      |
| <b>Examples</b>    | <pre>Set cal = pna.ActiveChannel.Calibrator moduleFound = cal.IsECALModuleFound(naECALModule_A)</pre>                                                                                                                               |
| <b>C++ Syntax</b>  | HRESULT get_IsECALModuleFound(tagNAECALModule moduleNumber, VARIANT_BOOL *bModuleFound);                                                                                                                                            |
| <b>Interface</b>   | Calibrator                                                                                                                                                                                                                          |

**LogMagnitudeOffset Property** OBSOLETE

**Description** **Note:** This property is replaced by [DoReceiverPowerCal Method](#).

**For Receiver Calibration** - Sets or returns the value to offset the normalized unratiod power measurement data. The unratiod power measurement is effectively calibrated to the power level specified by the value of LogMagnitudeOffset as soon as the [Normalization property](#) is set to ON after calling the [DataToDivisor](#) method.

To offset the data trace magnitude a specified value, use [MagnitudeOffset Property](#)

**VB Syntax** *meas.LogMagnitudeOffset = value*

**Variable** **(Type) - Description**

*meas* **(object)** - A [Measurement](#) object

*value* **(double)** - Offset value in dBm.

**Return Type** Double

**Default** 0

**Examples** `meas.LogMagnitudeOffset = -10 'Write (-10 dBm)`

```
calpower = meas.LogMagnitudeOffset 'Read
meas.DataToDivisor 'Store meas data as measurement divisor
meas.Normalize = 1 'Measurement is now calibrated to -10 dBm
```

**C++ Syntax** HRESULT put\_LogMagnitudeOffset(double newVal);  
 HRESULT get\_LogMagnitudeOffset(double \*pVal);

**Interface** IMeasurement



## Normalization Property **OBSOLETE**

---

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
|--------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Description</b> | <b>Note:</b> This property is replaced by <code>DoReceiverPowerCal</code> Method.<br><br>Sets or returns normalization ON or OFF for the measurement. Normalization is currently supported only on measurements of unratioed power for the purpose of performing a receiver power calibration. If this property is set to ON for a ratioed measurement (such as S-parameter), it will return an error. This property will also return an error when set to ON if the divisor buffer doesn't yet exist. |
| <b>VB Syntax</b>   | <code>meas.Normalization = value</code>                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Variable</b>    | <b>(Type) - Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <code>meas</code>  | <b>(object)</b> - A Measurement object                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <code>value</code> | <b>(boolean)</b><br>0 – Turns normalization OFF<br>1 – Turns normalization ON                                                                                                                                                                                                                                                                                                                                                                                                                          |
| <b>Return Type</b> | Boolean                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Default</b>     | 0 -OFF                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Examples</b>    | <pre>meas.Normalization = 1 'Write<br/><br/>normalized = meas.Normalization 'Read</pre>                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>C++ Syntax</b>  | <pre>HRESULT put_Normalization(VARIANT_BOOL bState);<br/>HRESULT get_Normalization(VARIANT_BOOL *bState);</pre>                                                                                                                                                                                                                                                                                                                                                                                        |
| <b>Interface</b>   | IMeasurement                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |

Read-only

## PortsNeedingDeltaMatch Property

---

**Description** Returns the port numbers for which delta match correction is required. 0 (zero) is returned if the Cal does NOT require Delta Match correction for one of the following reasons:

- The Cal does NOT involve Unknown Thru or TRL. You specify this using [ThruCalMethod Property](#).
- The Cal DOES involve Unknown Thru or TRL, but the delta match data can be calculated by the Unknown Thru or TRL Cal. [Learn how this is possible](#). However, you can force the Cal to use the Delta Match data from a Cal Set.

**VB Syntax** *value* = *guided*.PortsNeedingDeltaMatch

**Variable** **(Type) - Description**

*value* (Variant) Variable to store the returned list of port numbers.

*guided* [GuidedCalibration](#) (object)

**Return Type** Variant

**Default** Not Applicable

**Examples**


```
Dim ports As Variant
ports = guided.PortsNeedingDeltaMatch
```

**C++ Syntax** HRESULT get\_PortsNeedingDeltaMatch (VARIANT\* portList);

**Interface** IGuidedCalibration2

## Calculate:FSimulator:Balun Commands

### CALCulate:FSIMulator:BALun

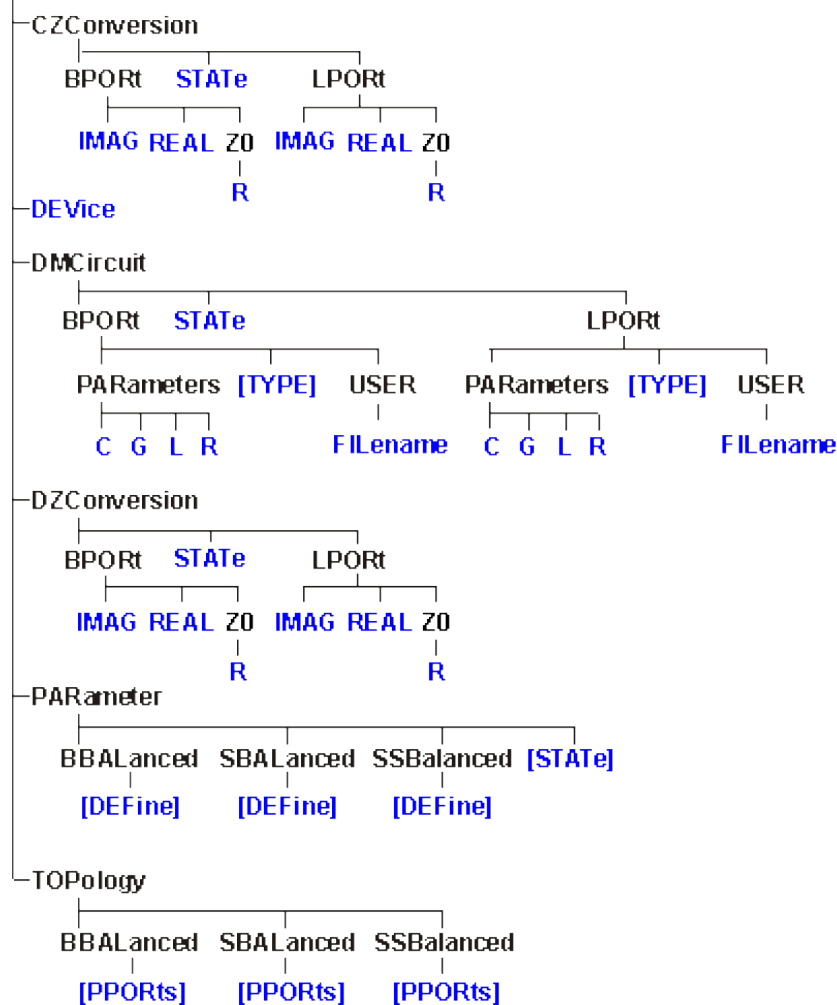

- Click on a blue keyword to view the command details.



- See a [List](#) of all commands in this block.
- [Learn about Balanced Measurements](#)

### Notes:

- [CALC:PAR:CAT?](#) alone can NOT be used to return a balanced measurement parameter. If a balanced measurement transform is being performed, then additional querying of the CALC:FSIM system is required to determine the balanced parameter type. [See an example.](#)
- CALCulate commands act on the selected measurement. You can select one measurement in each channel. Select the measurement for each channel using [CALC:PAR:SEL](#).
- **BPORT versus LPORt commands** - For each command in this subsystem that includes a BPORT keyword, there is an LPORt equivalent. The commands are identical except for the way in which the balanced / logical port numbers are specified:
  - The BPORT commands refer to the Balanced port number. There can only be up to two balanced ports.

This method is compatible with the ENA network analyzer.

- The LPORt commands refer to the Logical port number. A balanced port can appear as either logical port 1, 2, or 3. These are the references as they appear in the front-panel user interface.

| Topology          | Logical Port | Balanced Port |
|-------------------|--------------|---------------|
| Single-Bal        | 1            | N/A           |
|                   | 2            | 1             |
| Single-Single-Bal | 1            | N/A           |
|                   | 2            | N/A           |
|                   | 3            | 1             |
| Bal-Bal           | 1            | 1             |
|                   | 2            | 2             |

[Learn more about logical ports.](#)

### **CALCulate<cnum>:FSIMulator:BALun:CZConversion:BPORt<pnum>:IMAG <value>**

(Read-Write) Sets the imaginary part of the impedance value for the common port impedance conversion function.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

<value> Imaginary part of the Impedance value in Units. Choose a number between 0 and 1E18.

**Examples**

```
CALC:FSIM:BAL:CZC:BPOR:IMAG 0
calculate2:fsimulator:balun:czconversion:bport:imag 300
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:CZConversion:BPORt<pnum>:IMAG?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## CALCulate<cnum>:FSIMulator:BALun:CZConversion:BPORt<pnum>:REAL <value>

(Read-Write) Sets the real part of the impedance value for the common port impedance conversion function.

### Critical Note:

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Real part of the Impedance value in Units. Choose a number between 0 and 1E18.

#### Examples

```
CALC:FSIM:BAL:CZC:BPOR:REAL 25
calculate2:fsimulator:balun:czconversion:bport:real 50
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:CZConversion:BPORt<pnum>:REAL?

**Return Type** Numeric

**Overlapped?** No

**Default** See [Common Mode Port Z Conversion Default](#)

---

## CALCulate<cnum>:FSIMulator:BALun:CZConversion:BPORt<pnum>:Z0[:R] <value>

(Read-Write) Sets the real part of the impedance value for the common port impedance conversion function. Set either this single value or set the [real](#) and [imaginary](#) parts separately. The imaginary part is set to 0.0 using this command.

### Critical Note:

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Impedance value in ohms. Choose a number between 0 to 1E7.

**Examples**

```
CALC:FSIM:BAL:CZC:BPOR:Z0 50
calculate2:fsimulator:balun:czconversion:bport:z0:r 75
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:CZConversion:BPORt<pnum>:Z0[:R]?

**Return Type** Numeric

**Overlapped?** No

**Default** See [Common Mode Port Z Conversion Default](#)

---

### CALCulate<cnum>:FSIMulator:BALun:CZConversion:STATe <bool>

(Read-Write) Sets the common port impedance conversion function ON/OFF. Must also set the fixture simulator function to ON using [CALC:FSIM:STAT](#).

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<bool> State of common port impedance conversion function. Choose from

**OFF (or 0)** Conversion OFF

**ON (or 1)** Conversion ON

**Examples**

```
CALC:FSIM:BAL:CZC:STAT 1
calculate2:fsimulator:balun:czconversion:state off
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:CZConversion:STATe?

**Return Type** Boolean

**Overlapped?** No

**Default** Off

---

### CALCulate<cnum>:FSIMulator:BALun:CZConversion:LPORt<pnum>:IMAG <value>

(Read-Write) Sets the imaginary part of the impedance value for the common port impedance conversion function.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports 1, 2, or 3.

---

**Note:** See Balanced port versus Logical port.

---

<value> Imaginary part of the Impedance value in Units. Choose a number between 0 and 1E18.

**Examples**

```
CALC:FSIM:BAL:CZC:LPOR:IMAG 0
calculate2:fsimulator:balun:czconversion:lport:imag 300
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:CZConversion:LPORt<pnum>:IMAG?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**CALCulate<cnum>:FSIMulator:BALun:CZConversion:LPORt<pnum>:REAL <value>**

(Read-Write) Sets the real part of the impedance value for the common port impedance conversion function.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports 1, 2, or 3.

---

**Note:** See Balanced port versus Logical port.

---

<value> Real part of the Impedance value in Units. Choose a number between 0 and 1E18.

**Examples**

```
CALC:FSIM:BAL:CZC:LPOR:REAL 25
calculate2:fsimulator:balun:czconversion:lport:real 50
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:CZConversion:LPORt<pnum>:REAL?

**Return Type** Numeric

**Overlapped?** No

**Default** See [Common Mode Port Z Conversion Default](#)

---

### **CALCulate<cnum>:FSIMulator:BALun:CZConversion:LPORt<pnum>:Z0[:R] <value>**

(Read-Write) Sets the real part of the impedance value for the common port impedance conversion function. Set either this single value or set the real and imaginary parts separately. The imaginary part is set to 0.0 using this command.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports **1, 2, or 3**.

---

**Note:** See [Balanced port versus Logical port](#).

---

<value> Impedance value in ohms. Choose a number between 0 to 1E7.

**Examples**

```
CALC:FSIM:BAL:CZC:LPOR:Z0 50
calculate2:fsimulator:balun:czconversion:lport:z0:r 75
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:CZConversion:LPORt<pnum>:Z0[:R]?

**Return Type** Numeric

**Overlapped?** No

**Default** See [Common Mode Port Z Conversion Default](#)

---

### **CALCulate<cnum>:FSIMulator:BALun:DEVIce <char>**



(Read-Write) Selects the device type for the balanced measurement.

**Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<char> **SBALanced** - Single-ended - Balanced device (3 ports).

**BBALanced** - Balanced - Balanced device (4 ports).

**SSBALanced** - Single-ended - Single-ended - Balanced device (4 ports).

**Examples**

```
CALC:FSIM:BAL:DEV SSB
calculate2:fsimulator:balun:device bbal
```

**Query Syntax** CALCulate<num>:FSIMulator:BALun:DEVice?

**Return Type** Character

**Overlapped?** No

**Default** SBALanced

---

**CALCulate<num>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:C <value>**

(Read-Write) Sets the Capacitance value of the differential matching circuit.

**Critical Note:**

**Parameters**

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

<value> Capacitance value in farads. Choose a number between -1E18 to 1E18

**Examples**

```
CALC:FSIM:BAL:DMC:BPOR:PARAmeters:C 10E-6
calculate2:fsimulator:balun:dmcircuit:bport:parameters:c 1E-9
```

**Query Syntax** CALCulate<num>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:C?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:G <value>**

(Read-Write) Sets the Conductance value of the differential matching circuit.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Conductance value in siemens. Choose a number between -1E18 to 1E18.

**Examples**

```
CALC:FSIM:BAL:DMC:BPOR:PARAmeters:G 1E3
calculate2:fsimulator:balun:dmcircuit:bport:parameters:g 1E-3
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:G?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:L <value>**

(Read-Write) Sets the Inductance value of the differential matching circuit.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Inductance value in henries. Choose a number between -1E18 to 1E18.

**Examples**

```
CALC:FSIM:BAL:DMC:BPOR:PARAMeters:L 3E-3
calculate2:fsimulator:balun:dmcircuit:bport:parameters:lE-10
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:L?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:R <value>**

(Read-Write) Sets the Resistance value of the differential matching circuit.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Resistance value in ohms. Choose a number between -1E18 to 1E18.

**Examples**

```
CALC:FSIM:BAL:DMC:BPOR:PARAMeters:R 100
calculate2:fsimulator:balun:dmcircuit:bport:parameters:r 4E3
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:PARAmeters:R?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## **CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>[:TYPE] <char>**

(Read-Write) Sets the differential matching circuit type. To select a user-defined circuit, specify IN ADVANCE the 2-port touchstone filename with `CALC:FSIM:BAL:DMC:BPOR:USER:FILENAME`. If you do not specify the appropriate file and you select **USER**, an error occurs and **NONE** is automatically selected.

### **Critical Note:**

#### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<char> Circuit type. Choose from:

**NONE** - Specifies no-circuit.

**PLPC** - Specifies the circuit that consists of shunt L and shunt C.

**USER** - Specifies the user-defined circuit.

#### **Examples**

```
CALC:FSIM:BAL:DMC:BPOR2 PLPC
calculate2:fsimulator:balun:dmcircuit:bport1:type none
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:TYPE?

**Return Type** Character

**Overlapped?** No

**Default** PLPC

---

## **CALCulate<cnum>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:USER:FILENAME <string>**

(Read-Write) Specifies the 2-port touchstone file in which the information on the user-defined differential matching circuit is saved. Following this command, send `CALC:FSIM:BAL:DMC:BPOR2 USER`. If the specified file does not exist, an error occurs when you set the type of differential matching circuit to USER.

**Critical Note:**

**Parameters**

<cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.

<pnum> Balanced port number. Choose from ports 1 or 2.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<string> File name and extension (.s2P) of the differential matching circuit. Files are stored in the default folder "C:\Program Files\Agilent\Network Analyzer\Documents". To recall from a different folder, specify the full path name.

**Examples**

```
CALC:FSIM:BAL:DMC:BPOR:USER:FIL 'myfile.s2p'
calculate2:fsimulator:balun:dmcircuit:bport:user:filename
"C:\Program Files\Agilent\Network Analyzer\Documents\myFile.s2P"
```

**Query Syntax** CALCulate<cnun>:FSIMulator:BALun:DMCircuit:BPORt<pnum>:USER:FILEname?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

**CALCulate<cnun>:FSIMulator:BALun:DMCircuit:STATe <bool>**

(Read-Write) Sets the differential matching circuit embedding function ON/OFF. Must also set the fixture simulator function to ON using `CALC:FSIM:STAT`.

**Critical Note:**

**Parameters**

<cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.

<bool> State of differential matching circuit embedding function. Choose from  
**OFF (or 0)** Matching circuit OFF  
**ON (or 1)** Matching circuit ON

**Examples**

```
CALC:FSIM:BAL:DMC:STAT 1
calculate2:fsimulator:balun:dmcircuit:state off
```

---

|                           |                                                   |
|---------------------------|---------------------------------------------------|
| <b>Query Syntax</b>       | CALCulate<cnum>:FSIMulator:BALun:DMCircuit:STATe? |
| <b>Return Type</b>        | Boolean                                           |
| <b><u>Overlapped?</u></b> | No                                                |
| <b><u>Default</u></b>     | Off                                               |

---

### **CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:C <value>**

(Read-Write) Sets the Capacitance value of the differential matching circuit.

**Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
  - <pnum> Logical port number. Choose from logical ports **1, 2, or 3**.
- 
- Note:** See [Balanced port versus Logical port](#).
- 
- <value> Capacitance value in farads. Choose a number between -1E18 to 1E18

**Examples**

```
CALC:FSIM:BAL:DMC:LPOR:PARAmeters:C 10E-6
calculate2:fsimulator:balun:dmcircuit:lport:parameters:c 1E-9
```

|                           |                                                                      |
|---------------------------|----------------------------------------------------------------------|
| <b>Query Syntax</b>       | CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:C? |
| <b>Return Type</b>        | Numeric                                                              |
| <b><u>Overlapped?</u></b> | No                                                                   |
| <b><u>Default</u></b>     | 0                                                                    |

---

### **CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:G <value>**

(Read-Write) Sets the Conductance value of the differential matching circuit.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports 1, 2, or 3.

---

**Note:** See Balanced port versus Logical port.

---

<value> Conductance value in siemens. Choose a number between -1E18 to 1E18.

**Examples**

```
CALC:FSIM:BAL:DMC:LPOR:PARAMeters:G 1E3
calculate2:fsimulator:balun:dmcircuit:lport:parameters:g 1E-3
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:G?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

**CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:L <value>**

(Read-Write) Sets the Inductance value of the differential matching circuit.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports 1, 2, or 3.

---

**Note:** See Balanced port versus Logical port.

---

<value> Inductance value in henries. Choose a number between -1E18 to 1E18.

**Examples**

```
CALC:FSIM:BAL:DMC:LPOR:PARAMeters:L 3E-3
calculate2:fsimulator:balun:dmcircuit:lport:parameters:lE-10
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:L?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:R <value>**

(Read-Write) Sets the Resistance value of the differential matching circuit.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports **1, 2, or 3**.

---

**Note:** See Balanced port versus Logical port.

---

<value> Resistance value in ohms. Choose a number between -1E18 to 1E18.

**Examples**

```
CALC:FSIM:BAL:DMC:LPOR:PARAmeters:R 100
calculate2:fsimulator:balun:dmcircuit:lport:parameters:r 4E3
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:PARAmeters:R?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>[:TYPE] <char>**

(Read-Write) Sets the differential matching circuit type. To select a user-defined circuit, specify IN ADVANCE the 2-port touchstone filename with CALC:FSIM:BAL:DMC:LPOR:USER:FILENAME. If you do not specify the appropriate file and you select **USER**, an error occurs and NONE is automatically selected.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports **1, 2, or 3**.

---

**Note:** See Balanced port versus Logical port.

---



<char> Circuit type. Choose from:  
**NONE** - Specifies no-circuit.  
**PLPC** - Specifies the circuit that consists of shunt L and shunt C.  
**USER** - Specifies the user-defined circuit.

**Examples**

```
CALC:FSIM:BAL:DMC:LPOR2 PLPC
calculate2:fsimulator:balun:dmcircuit:lport1:type none
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:TYPE?

**Return Type** Character

**Overlapped?** No

**Default** PLPC

---

**CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:USER:FILEname <string>**

(Read-Write) Specifies the 2-port touchstone file in which the information on the user-defined differential matching circuit is saved. Following this command, send CALC:FSIM:BAL:DMC:BPOR2 USER. If the specified file does not exist, an error occurs when you set the type of differential matching circuit to USER.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports 1, 2, or 3.

---

**Note:** See Balanced port versus Logical port.

---

<string> File name and extension (.s2P) of the differential matching circuit. Files are stored in the default folder "C:\Program Files\Agilent\Network Analyzer\Documents". To recall from a different folder, specify the full path name.

**Examples**

```
CALC:FSIM:BAL:DMC:LPOR:USER:FIL 'myfile.s2p'
calculate2:fsimulator:balun:dmcircuit:lport:user:filename
"C:\Program Files\Agilent\Network Analyzer\Documents\myFile.s2P"
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DMCircuit:LPORt<pnum>:USER:FILEname?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

## CALCulate<cnum>:FSIMulator:BALun:DZConversion:BPORt<pnum>:IMAG <value>

(Read-Write) Sets the imaginary part of the impedance value for the differential port impedance conversion function.

### Critical Note:

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Imaginary part of the Impedance value in Units. Choose a number between 0 and 1E18.

#### Examples

```
CALC:FSIM:BAL:DZC:BPOR:IMAG 0
calculate2:fsimulator:balun:dczconversion:bport:imag 300
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DZConversion:BPORt<pnum>:IMAG?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## CALCulate<cnum>:FSIMulator:BALun:DZConversion:BPORt<pnum>:REAL <value>

(Read-Write) Sets the real part of the impedance value for the differential port impedance conversion function.

### Critical Note:

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Real part of the Impedance value in Units. Choose a number between 0 and 1E18

#### Examples

```
CALC:FSIM:BAL:DZC:BPOR:REAL 50
calculate2:fsimulator:balun:dczconversion:bport:real 75
```

---

|                     |                                                                 |
|---------------------|-----------------------------------------------------------------|
| <b>Query Syntax</b> | CALCulate<cnum>:FSIMulator:BALun:DZConversion:BPORt<pnum>:REAL? |
| <b>Return Type</b>  | Numeric                                                         |
| <b>Overlapped?</b>  | No                                                              |
| <b>Default</b>      | See <a href="#">Differential Port Z Conversion Default</a>      |

---

## CALCulate<cnum>:FSIMulator:BALun:DZConversion:BPORt<pnum>:Z0[:R] <value>

(Read-Write) Sets the impedance value for the differential port impedance conversion function. Set either this single value or set the [real](#) and [imaginary](#) parts separately. The imaginary part is set to 0.0 using this command.

### **Critical Note:**

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Balanced port number. Choose from ports **1** or **2**.

---

**Note:** The numbering of logical ports is different from balanced ports. This command works the same as the ENA network analyzer. If there is only one balanced port, it is Balanced Port 1, regardless of the port mapping assignment. [Learn more.](#)

---

<value> Impedance value in ohms. Choose a number between 0 to 1E7

#### Examples

```
CALC:FSIM:BAL:DZC:BPOR:Z0 50
calculate2:fsimulator:balun:dzconversion:bport:z0:r 75
```

|                     |                                                                   |
|---------------------|-------------------------------------------------------------------|
| <b>Query Syntax</b> | CALCulate<cnum>:FSIMulator:BALun:DZConversion:BPORt<pnum>:Z0[:R]? |
| <b>Return Type</b>  | Numeric                                                           |
| <b>Overlapped?</b>  | No                                                                |
| <b>Default</b>      | See <a href="#">Differential Port Z Conversion Default</a>        |

---

## CALCulate<cnum>:FSIMulator:BALun:DZConversion:STATE <bool>

(Read-Write) Sets the differential port impedance conversion function ON/OFF. Must also set the fixture simulator function to ON using CALC:FSIM:STAT.

**Critical Note:**

**Parameters**

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <bool> State of the differential port impedance conversion function. Choose from  
**OFF (or 0)** Differential port impedance conversion OFF  
**ON (or 1)** Differential port impedance conversion ON

**Examples**

```
CALC:FSIM:BAL:DZC:STAT 1
calculate2:fsimulator:balun:dzconversion:state off
```

**Query Syntax** CALCulate<num>:FSIMulator:BALun:DZConversion:STATe?

**Return Type** Boolean

**Overlapped?** No

**Default** Off

---

**CALCulate<num>:FSIMulator:BALun:DZConversion:LPORt<pnum>:IMAG <value>**

(Read-Write) Sets the imaginary part of the impedance value for the differential port impedance conversion function.

**Critical Note:**

**Parameters**

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <pnum> Logical port number. Choose from logical ports **1, 2, or 3**.  

---

**Note:** See Balanced port versus Logical port.

---
- <value> Imaginary part of the Impedance value in Units. Choose a number between 0 and 1E18.

**Examples**

```
CALC:FSIM:BAL:DZC:LPOR:IMAG 0
calculate2:fsimulator:balun:dczconversion:lport:imag 300
```

**Query Syntax** CALCulate<num>:FSIMulator:BALun:DZConversion:LPORt<pnum>:IMAG?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:FSIMulator:BALun:DZConversion:LPORt<pnum>:REAL <value>**

(Read-Write) Sets the real part of the impedance value for the differential port impedance conversion function.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports 1, 2, or 3.

---

**Note:** See [Balanced port versus Logical port](#).

---

<value> Real part of the Impedance value in Units. Choose a number between 0 and 1E18

**Examples**

```
CALC:FSIM:BAL:DZC:LPOR:REAL 50
calculate2:fsimulator:balun:dzconversion:lport:real 75
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DZConversion:LPORt<pnum>:REAL?

**Return Type** Numeric

**Overlapped?** No

**Default** See [Differential Port Z Conversion Default](#)

---

### **CALCulate<cnum>:FSIMulator:BALun:DZConversion:LPORt<pnum>:Z0[:R] <value>**

(Read-Write) Sets the impedance value for the differential port impedance conversion function. Set either this single value or set the [real](#) and [imaginary](#) parts separately. The imaginary part is set to 0.0 using this command.

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<pnum> Logical port number. Choose from logical ports 1, 2, or 3.

---

**Note:** See [Balanced port versus Logical port](#).

---

<value> Impedance value in ohms. Choose a number between 0 to 1E7

**Examples**

```
CALC:FSIM:BAL:DZC:LPOR:Z0 50
calculate2:fsimulator:balun:dzconversion:lport:z0:r 75
```

---

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:DZConversion:LPORT<pnum>:Z0[:R]?  
**Return Type** Numeric  
**Overlapped?** No  
**Default** See [Differential Port Z Conversion Default](#)

---

**CALCulate<cnum>:FSIMulator:BALun:PARAMeter<n>:BBALanced[:DEFine] <char>**

(Read-Write) For a Balanced - Balanced device type, selects the measurement parameter for the specified trace. Set device type using [CALC:FSIM:BAL:DEV](#)

**Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <n> Trace number on the specified channel <cnum>
- <char> Balanced- Balanced Measurement parameter. Choose from:

|       |       |                     |       |
|-------|-------|---------------------|-------|
| Sdd11 | Sdd12 | Sdc11               | Sdc12 |
| Sdd21 | Sdd22 | Sdc21               | Sdc22 |
| Scd11 | Scd12 | Scd11               | Scd12 |
| Scd21 | Scd22 | Scd21               | Scd22 |
| lmb1  | lmb2  | CMRR -(Sdd21/Scd21) |       |

**Examples**

```
CALC:FSIM:BAL:PAR:BBAL SDD12
calculate1:fsimulator:balun: parameter2:bbalanced:define cmrr
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:PARAMeter<n>:BBALanced[:DEFine]?  
**Return Type** Character  
**Overlapped?** No  
**Default** Sdd11

---

**CALCulate<cnum>:FSIMulator:BALun:PARAMeter<n>:SBALanced[:DEFine] <char>**

(Read-Write) For a Single-ended - Balanced device type, selects the measurement parameter for the specified trace. Set device type using CALC:FSIM:BAL:DEV

**Critical Note:**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <n> Trace number on the specified channel <cnum>
- <char> Single-ended - Balanced Measurement parameter. Choose from:

|       |                        |                        |
|-------|------------------------|------------------------|
| Sss11 | Ssd12                  | Scs12                  |
| Sds21 | Sdd22                  | Sdc22                  |
| Scs21 | Scd22                  | Sc22                   |
| Imb   | CMRR1<br>(Sds21/Scs21) | CMRR2<br>(Ssd12/Scs12) |

**Examples**

```
CALC:FSIM:BAL:PAR:SBAL SSD12
calculate1:fsimulator:balun: parameter2:sbalanced:define imb
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:PARAmeter<n>:SBALanced[:DEFine]?

**Return Type** Character

**Overlapped?** No

**Default** Sss11

**CALCulate<cnum>:FSIMulator:BALun:PARAmeter<n>:SSBalanced[:DEFine] <char>**

(Read-Write) For a Single-ended - Single-ended - Balanced device type, selects the measurement parameter for the specified trace. Set device type using CALC:FSIM:BAL:DEV

**Critical Note:**

**Parameters**

<cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.

<n> Trace number on the specified channel <cnun>

<char> Single-ended - Single-ended - Balanced Measurement parameter. Choose from:

|       |       |                        |                        |
|-------|-------|------------------------|------------------------|
| Sss11 | Sss12 | Ssd13                  | Ssc13                  |
| Sss21 | Sss22 | Ssd23                  | Ssc23                  |
| Sds31 | Sds32 | Sdd33                  | Sdc33                  |
| Scs31 | Scs32 | Scd33                  | Sc33                   |
| Imb1  | Imb2  | CMRR1<br>(Sds31/Scs31) | CMRR2<br>(Sds32/Scs32) |

**Examples**

```
CALC:FSIM:BAL:PAR:SSB SSD23
calculatel:fsimulator:balun: parameter2:ssbalanced:define imb1
```

**Query Syntax** CALCulate<cnun>:FSIMulator:BALun:PARAmeter<n>:SSBalanced[:DEFine]?

**Return Type** Character

**Overlapped?** No

**Default** Sss11

**CALCulate<cnun>:FSIMulator:BALun:PARAmeter<n>:STATe <bool>**



(Read-Write) Turns balanced transform ON and OFF.

**Critical Note:**

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <n> Trace number on the specified channel <cnun>
- <bool> State of balanced transform. Choose from  
**OFF (or 0)** Balanced Transform OFF  
**ON (or 1)** Balanced Transform ON

**Examples**

```
CALC:FSIM:BAL:PAR:STAT 1
calculate1:fsimulator:balun:parameter2:state off
```

**Query Syntax** CALCulate<cnun>:FSIMulator:BALun:PARAmeter<n>:STATe?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF

**CALCulate<cnun>:FSIMulator:BALun:TOPology:BBALanced[:PPORts]  
<p1Pos>,<p1Neg>,<p2Pos>,<p2Neg>**


(Read-Write) For a Balanced - Balanced device type, maps the PNA ports to the DUT ports.

Set the Balanced - Balanced device type using CALC:FSIM:BAL:DEV

**Critical Note:**

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <p1Pos> PNA port number that connects to each of the following DUT ports:
- <p1Neg>
- <p2Pos>
- <p2Neg>

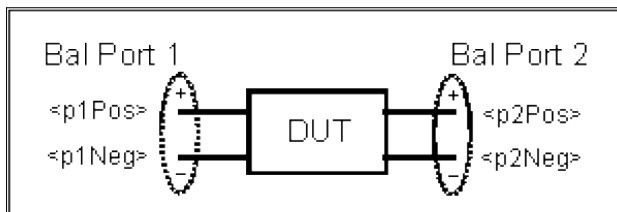

**Examples**

```
CALC:FSIM:BAL:TOP:BBAL 1,2,3,4
calculate1:fsimulator:balun: topology:bbalanced:pports 4,3,2,1
```

---

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:TOPology:BBALanced[:PPORts]?

**Return Type** Numeric - Returns four numbers separated by commas.

**Overlapped?** No

**Default** Not Applicable

---

## CALCulate<cnum>:FSIMulator:BALun:TOPology:SBALanced[:PPORts] <se>,<bPos>,<bNeg>

(Read-Write) For a Single-ended - Balanced device type, maps the PNA ports to the DUT ports.

Set the Single-ended - Balanced device type using CALC:FSIM:BAL:DEV

### Critical Note:


#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<se> PNA port number that connects to each of the following DUT ports:

<bPos>

<bNeg>

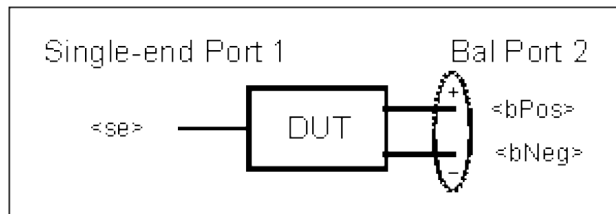

#### Examples

```
CALC:FSIM:BAL:TOP:SBAL 1,2,3
```

```
calculatel:fsimulator:balun: topology:sbalanced:pports 4,3,2
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:TOPology:SBALanced[:PPORts]?

**Return Type** Numeric - Returns three numbers separated by commas.

**Overlapped?** No

**Default** Not Applicable

---

## CALCulate<cnum>:FSIMulator:BALun:TOPology:SSBALanced[:PPORts] <se1>,<se2>,<bPos>,<bNeg>


(Read-Write) For a Single-ended - Single-ended - Balanced device type, maps the PNA ports to the DUT ports. Set the Single-ended - Single-ended - Balanced device type using CALC:FSIM:BAL:DEV

**Critical Note:**

**Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<se1> PNA port number that connects to each of the following DUT ports:

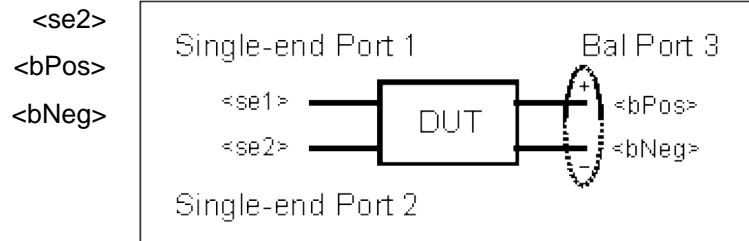

**Examples**

```
CALC:FSIM:BAL:TOP:SSB 1,2,3,4
calculate1:fsimulator:balun:topology:ssbalanced:pports 4,3,2,1
```

**Query Syntax** CALCulate<cnum>:FSIMulator:BALun:TOPology:SSBalanced[:PPORts]?

**Return Type** Numeric - Returns four numbers separated by commas.


**Overlapped?** No

**Default** Not Applicable

## Calculate:FSimulator:Embed Commands

---

Specifies settings for embedding and de-embedding balanced (4-port) fixturing circuits.

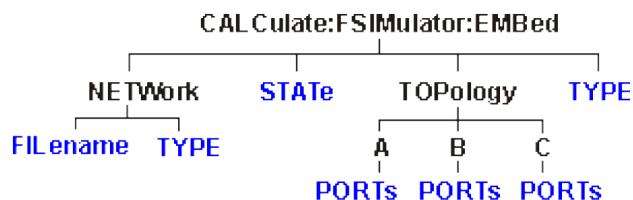

- Click a **blue** keyword to view the command details.
  - See a [List](#) of all SCPI commands.
- 

### CALCulate<cnum>:FSIMulator:EMBed:NETWork<n>:FILEname <string>


(Read-Write) Specifies the 4-port touchstone file (\*.s4p) in which the network to embed or de-embed resides. Following this command, send CALC:FSIM:EMB:NETW:TYPE. If the specified file does not exist, an error occurs when type command is sent.

[Learn about 4-port network embedding.](#)

#### Parameters

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <n> Network position. Choose from 1 or 2.
- <string> File name and extension (.s4P) of the circuit. Files are stored in the default folder "C:\Program Files\Agilent\Network Analyzer\Documents". To recall from a different folder, specify the full path name.

#### Examples



```
10 calculate2:fsimulator:embed:network2:filename "C:\Program
Files\Agilent\Network Analyzer\Documents\myFile.s4P"
20 calculate2:fsimulator:embed:network2:type embed
```

**Query Syntax** CALCulate<cnum>:FSIMulator:EMBed:NETWork<n>:FILEname?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

### CALCulate<cnum>:FSIMulator:EMBed:NETWork<n>:TYPE <char>

(Read-Write) Specify the type of processing to take place on the specified 4-port network. First specify the network filename with CALC:FSIM:EMB:NETW:FIL.

Learn about 4-port network embedding.

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<n> Network position. Choose from **1** or **2**.

<char> Processing type. Choose from :

**NONE** - The same as disabling.

**EMBed** - Add Network circuit.

**DEEMbed** - Remove Network circuit.

#### Example

```
10 CALC:FSIM:EMB:NETW2:FIL 'myFile.s4p'
20 CALC:FSIM:EMB:NETW2:TYPE EMBed
```

**Query Syntax** CALCulate<cnum>:FSIMulator:EMBed:NETWork<n>:TYPE?

**Return Type** Character

**Overlapped?** No

**Default** NONE

---

### CALCulate<cnum>:FSIMulator:EMBed:STATE <bool>

(Read-Write) Turns ON or OFF 4-port Network Embedding/De-embedding for all ports on the specified channel.

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<bool> Choose from:

**ON or 1** - Turns 4-port Network Embedding/De-embedding ON

**OFF or 0** - Turns 4-port Network Embedding/De-embedding OFF

#### Examples

```
CALC:FSIM:EMB:STAT 1
calculate2:fsimulator:embed:state 0
```

**Query Syntax** CALCulate<cnum>:FSIMulator:EMBed:STATE?

**Return Type** Boolean


**Overlapped?** No

**Default** OFF

---

**CALCulate<cnum>:FSIMulator:EMBed:TOPology:A:PORTs <p1>,<p2>**

(Read-Write) Specifies the PNA port connections when topology A is selected. Specify topology using CALC:FSIM:EMBed:TYPE.

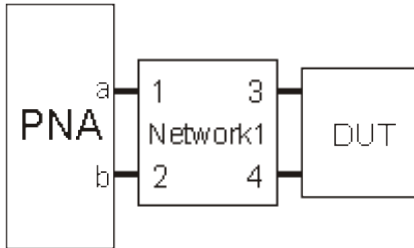

**Topology A**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <p1> PNA Port number assigned to **a** in above graphic.
- <p2> PNA Port number assigned to **b** in above graphic.

**Examples**

```
CALC:FSIM:EMB:TOP:A:PORT 2,1
calculate2:fsimulator:embed:topology:a:ports 1,2
```

**Query Syntax** CALCulate<cnum>:FSIMulator:EMBed:TOPology:A:PORTs?

**Return Type** Numeric


**Overlapped?** No

**Default** 1,2

---

**CALCulate<cnum>:FSIMulator:EMBed:TOPology:B:PORTs <p1>,<p2>,<p3>**

(Read-Write) Specifies the PNA port connections when topology B is selected. Specify topology using CALC:FSIM:EMBed:TYPE.

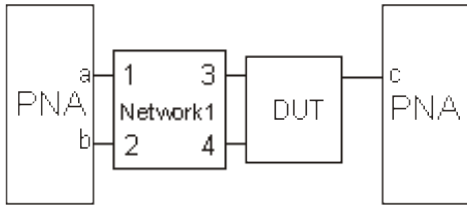

**Topology B**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <p1> PNA Port number assigned to **a** in above graphic.
- <p2> PNA Port number assigned to **b** in above graphic.
- <p3> PNA Port number assigned to **c** in above graphic.

**Examples**

```
CALC:FSIM:EMB:TOP:B:PORT 2,1,4
calculate2:fsimulator:embed:topology:b:ports 1,2,3
```

**Query Syntax** CALCulate<cnum>:FSIMulator:EMBed:TOPology:B:PORTs?


**Return Type** Numeric

**Overlapped?** No

**Default** 1,2,3

**CALCulate<cnum>:FSIMulator:EMBed:TOPology:C:PORTs <p1>,<p2>,<p3>,<p4>**

(Read-Write) Specifies the PNA port connections when topology C is selected. Specify topology using CALC:FSIM:EMBed:TYPE.

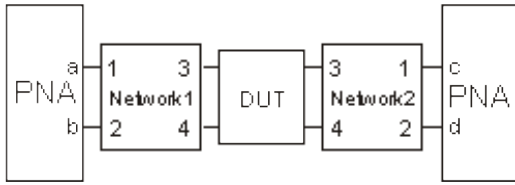

**Topology C**

**Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <p1> PNA Port number assigned to **a** in above graphic.
- <p2> PNA Port number assigned to **b** in above graphic.
- <p3> PNA Port number assigned to **c** in above graphic.
- <p4> PNA Port number assigned to **d** in above graphic.

**Examples**

```
CALC:FSIM:EMB:TOP:C:PORT 2,1,4,3
calculate2:fsimulator:embed:topology:c:ports 1,2,3,4
```

**Query Syntax** CALCulate<cnum>:FSIMulator:EMBed:TOPology:C:PORTs?

**Return Type** Numeric

**Overlapped?** No

**Default** 1,2,3,4

**CALCulate<cnum>:FSIMulator:EMBed:TYPE <char>**



(Read-Write) Specifies the PNA / DUT topology. [Learn more about these and other PNA/DUT configurations.](#)

### Parameters

<num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.

<char> PNA / DUT topology. Choose from:

- **A** - 2 PNA/DUT Ports
- **B** - 3 PNA/DUT Ports
- **C** - 4 PNA/DUT Ports

Click links to see topologies and port assignment commands.

### Examples

```
CALC:FSIM:EMB:TYPE A
calculate2:fsimulator:embed:type c
```

**Query Syntax** CALCulate<num>:FSIMulator:EMBed:TYPE?

**Return Type** Character


**Overlapped?** No

**Default** A

## Calculate:FSimulator:SEnDed Commands

---

Specifies settings for embedding and de-embedding **Single-Ended** (2-port) fixturing circuits.

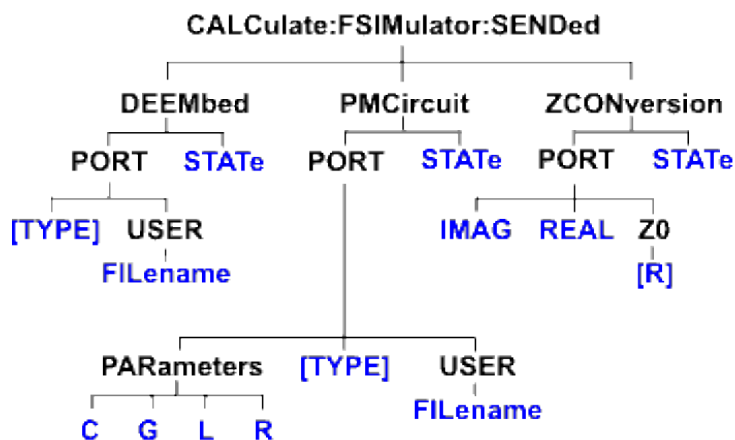

- Click on a blue keyword to view the command details.
- See a [List](#) of all commands in this block.
- [Learn about Fixturing](#)
- [Set Port Extensions with SCPI](#)

---

**Note:** CALC:FSIM commands affect ALL measurements on the specified channel.

---

### CALCulate<cnum>:FSIMulator:SEnDed:DEEMbed:PORT<n>[:TYPE] <char>

(Read-Write) Select whether or not to load a 2-port De-embedding circuit model for the specified port number. Circuit model USER is valid when an associated .s2p file is specified with [CALC:FSIM:SEND:DEEM:PORT1:USER:FILENAME](#).

---

**Note:** This command affects ALL measurements on the specified channel.



#### Parameters

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <port> Port number to receive circuit model.
- <char> Choose from:
- NONE** - Port does not have a circuit model.
  - USER** - Circuit model for the port will be loaded from PNA drive.

#### Examples

```
CALC:FSIM:SEND:DEEM:PORT1 USER
calculate2:fsimulator:sended:deembedded:port2:type none
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SEnDed:DEEMbed:PORT<n>[:TYPE]?

**Return Type** Character

**Overlapped?** No

**Default** None

---

## **CALCulate<cnum>:FSIMulator:SENDEd:DEEMbed:PORT<n>:USER:FILEname <string>**

(Read-Write) Specifies the filename of the circuit model to be used for de-embedding. Circuit model is applied when both CALC:FSIM:SEND:DEEM:PORT1 USER is selected and the filename is specified with this command.

**Note:** This command affects ALL measurements on the specified channel.

---

### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<port> Port number to receive circuit model.

<string> File name and extension (.s2P) of the de-embedding circuit.

Files are stored in the default folder "C:\Program Files\Agilent\Network Analyzer\Documents

To recall from a different folder, specify the full path name.

### **Examples**

```
CALC:FSIM:SEND:DEEM:PORT1:USER:FILE 'myFile.s2P'
calculate2:fsimulator:deembed:port2:user:file "C:\Program
Files\Agilent\Network Analyzer\Documents\myFile.s2P"
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:DEEMbed:PORT<n>:USER:FILEname?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

## **CALCulate<cnum>:FSIMulator:SENDEd:DEEMbed:PORT<n>:STATe <bool>**

(Read-Write) Turns de-embedding ON or OFF for all ports on the specified channel.

---

**Note:** This command affects ALL measurements on the specified channel.

---

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <port> Port number to receive circuit model.
- <bool> Choose from:
  - ON** or **1** - Turns de-embedding ON
  - OFF** or **0** - Turns de-embedding OFF

**Examples**

```
CALC:FSIM:SEND:DEEM:PORT1:STAT 1
calculate2:fsimulator:sended:deembed:port2:state 0
```

**Query Syntax** CALCulate<cnun>:FSIMulator:SENDEd:DEEMbed:PORT<n>:STATe?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF

---

**CALCulate<cnun>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:C <value>**

(Read-Write) Sets and returns the Capacitance, 'C' value for the specified port number.

---

**Note:** This command affects ALL measurements on the specified channel.

---

**Parameters**

- <cnun> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnun> is set to 1.
- <port> Port number to receive value.
- <value> Capacitance value in farads. Choose a value between -1E18 to 1E18

**Examples**

```
CALC:FSIM:SEND:PMC:PORT1:PAR:C 0.00002
calculate2:fsimulator:sended:pmcircuit:port2:parameters:c
0.00003
```

**Query Syntax** CALCulate<cnun>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:C?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:G <value>**

(Read-Write) Sets and returns the Conductance, 'G' value for the specified port number.

**Note:** This command affects ALL measurements on the specified channel.

---

#### **Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <port> Port number to receive value.
- <value> Conductance value in siemens. Choose a value between -1E18 to 1E18

#### **Examples**

```
CALC:FSIM:SEND:PMC:PORT1:PAR:G 0.00002
calculate2:fsimulator:sended:pmcircuit:port2:parameters:g
0.00003
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:G?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:L <value>**

(Read-Write) Sets and returns the Inductance, 'L' value for the specified port number.

**Note:** This command affects ALL measurements on the specified channel.

---

#### **Parameters**

- <cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.
- <port> Port number to receive value.
- <value> Inductance value in henries. Choose a value between -1E18 to 1E18

#### **Examples**

```
CALC:FSIM:SEND:PMC:PORT1:PAR:L 0.00002
calculate2:fsimulator:sended:pmcircuit:port2:parameters:l
0.00003
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:L?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## **CALCulate<cnum>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:R <value>**

(Read-Write) Sets and returns the Resistance, 'R' value for the specified port number.

**Note:** This command affects ALL measurements on the specified channel.

---

### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<port> Port number to receive value.

<value> Resistance value in ohms. Choose a value between -1E18 to 1E18

### **Examples**

```
CALC:FSIM:SEND:PMC:PORT1:PAR:R 0.00002
calculate2:fsimulator:sended:pmcircuit:port2:parameters:r
0.00003
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:PMCircuit:PORT<n>:PARAmeters:R?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

## **CALCulate<cnum>:FSIMulator:SENDEd:PMCircuit:PORT<n>[:TYPE] <char>**

(Read-Write) Select whether or not to load a 2 port matching circuit model for the specified port number. Circuit model USER is valid when an associated .s2p file is specified with CALC:FSIM:SEND:PMC:PORT1:USER:FILE

**Note:** This command affects ALL measurements on the specified channel.

---

### Parameters

- <num> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <num> is set to 1.
- <port> Port number to receive circuit model.
- <char> Circuit model. Choose from
- NONE** No circuit model
  - SLPC** Series L - Parallel C
  - PCSL** Parallel C - Series L
  - PLSC** Parallel L - Series C
  - SCPL** Series C - Parallel L
  - PLPC** Parallel L - Parallel C
  - USER** Load S2P file

### Examples

```
CALC:FSIM:SEND:PMC:PORT1:USER
calculate2:fsimulator:sended:pmcircuit:port2:type slpc
```

**Query Syntax** CALCulate<num>:FSIMulator:SENDEd:PMCircuit:PORT<n>[:TYPE]?

**Return Type** Character

**Overlapped?** No

**Default** None - No circuit model

---

**CALCulate<num>:FSIMulator:SENDEd:PMCircuit:PORT<n>:USER:FILEname <string>**

(Read-Write) Specifies the filename of the circuit model to be used for port matching. Circuit model is applied when both `CALC:FSIM:SEND:PMC:PORT1 USER` is selected and the filename is specified with this command.

---

**Note:** This command affects ALL measurements on the specified channel.

---

### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<port> Port number to receive circuit model.

<string> File name and extension (.s2P) of the de-embedding circuit.

Files are stored in the default folder "C:\Program Files\Agilent\Network Analyzer\Documents

To recall from a different folder, specify the full path name.

### Examples

```
CALC:FSIM:SEND:PMC:PORT1:USER:FILE 'myFile.s2P'
calculate2:fsimulator:pmcircuit:port2:user:file "C:\Program
Files\Agilent\Network Analyzer\Documents\myFile.s2P"
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDED:PMCircuit:PORT<n>:USER:FILENAME?

**Return Type** String

**Overlapped?** No

**Default** Not Applicable

---

## CALCulate<cnum>:FSIMulator:SENDED:PMCircuit:STATE <bool>

(Read-Write) Turns Port Matching ON or OFF for all ports on the specified channel.

---

**Note:** This command affects ALL measurements on the specified channel.

---

### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<bool> Choose from:

**ON or 1** - Turns Port Matching ON

**OFF or 0** - Turns Port Matching OFF

### Examples

```
CALC:FSIM:SEND:PMC:STAT 1
calculate2:fsimulator:sended:pmcircuit:state 0
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDED:PMCircuit:STATE?

**Return Type** Boolean



**Overlapped?** No

**Default** OFF

---

### **CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:PORT<n>:IMAG <value>**

(Read-Write) Sets and returns the Imaginary portion of the impedance value for the specified single-ended port. Use CALC:FSIM:SEND:ZCON:PORT:REAL to set the real value. Or use CALC:FSIM:SEND:ZCON:PORT:Z0 to set both values together.

**Note:** This command affects ALL measurements on the specified channel.

---

#### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<n> Port number to receive value.

<value> Imaginary impedance value. Choose a value between -1E18 and 1E18

#### **Examples**

```
CALC:FSIM:SEND:ZCON:PORT1:IMAG 75
calculate2:fsimulator:sended:zconversion:port2:imag 150
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:PORT<n>:IMAG?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

---

### **CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:PORT<n>:REAL <value>**

(Read-Write) Sets and returns the Real portion of the impedance value for the specified single-ended port. Use CALC:FSIM:SEND:ZCON:PORT:IMAG to set the imaginary value. Or use CALC:FSIM:SEND:ZCON:PORT:Z0 to set both values together.

---

**Note:** This command affects ALL measurements on the specified channel.

---

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<n> Port number to receive value.

<value> Real Impedance value in ohms. Choose a value between 0 to 1E7

#### Examples

```
CALC:FSIM:SEND:ZCON:PORT1:REAL 51
calculate2:fsimulator:sended:zconversion:port2:real 75
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:PORT<n>:REAL?

**Return Type** Numeric

**Overlapped?** No

**Default** 50

---

### **CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:PORT<n>:Z0[:R] <value>**

(Read-Write) Sets and returns the Real portion of the impedance value for the specified single-ended port. The imaginary portion is automatically set to 0.0.

To set both values separately, use CALC:FSIM:SEND:ZCON:PORT:REAL and CALC:FSIM:SEND:ZCON:PORT:IMAG.

---

**Note:** This command affects ALL measurements on the specified channel.

---

#### Parameters

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<n> Port number to receive value.

<value> Port Impedance value in ohms. Choose a value between 0 to 1E7

#### Examples

```
CALC:FSIM:SEND:ZCON:PORT1:Z0 51
calculate2:fsimulator:sended:zconversion:port2:z0:r 75
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:PORT<n>:Z0[:R]?

**Return Type** Numeric

**Overlapped?** No

**Default** 50

---

## **CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:STATe <bool>**

(Read-Write) Turns Port Impedance ON or OFF for all ports on the specified channel.

**Note:** This command affects ALL measurements on the specified channel.

---

### **Parameters**

<cnum> Channel number of the measurement. There must be a selected measurement on that channel. If unspecified, <cnum> is set to 1.

<bool> Choose from:

**ON** or **1** - Turns Port Impedance ON

**OFF** or **0** - Turns Port Impedance OFF

### **Examples**

```
CALC:FSIM:SEND:ZCON:STAT 1
calculate2:fsimulator:sended:zconversion:state 0
```

**Query Syntax** CALCulate<cnum>:FSIMulator:SENDEd:ZCONversion:STATe?

**Return Type** Boolean

**Overlapped?** No


**Default** OFF

---

## Sense:Multiplexer Commands

---

Controls the E5091A Test Set.

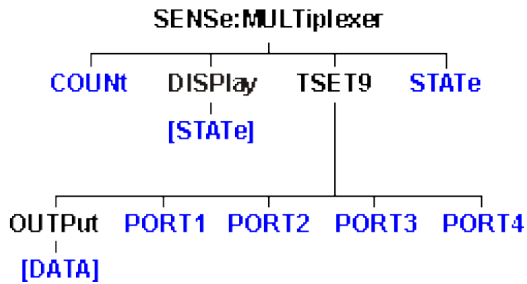

- Click on a blue keyword to view the command details.
  - See a [List](#) of all commands in this block.
  - [Learn about E5091A Test Set Control](#)
- 

### SENSe:MUlTIpLExer<id>:COUnT?

(Read-Only) Reads the number of ports (7 or 9) of the specified E5091A. Returns 0 if no test set is connected.

#### Parameters

<id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)

#### Examples

```
SENSe:MUlT1:COUnT?
sense:multiplexer2:count?
```

**Overlapped?** No

**Default** Not Applicable

---

### SENSe:MUlTIpLExer<id>:DISPly[:STATe] <bool>

(Read-Write) Turns ON and OFF the display of the current switch states of the specified E5091A.

**Parameters**

- <id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)
- <bool> ON(1) Turns ON the display.  
OFF (0) Turns OFF the display.

**Examples**

```
SENS:MULT1:DISP 1
sense:multiplexer2:display:state on
```

**Query Syntax** SENSE:MULTiplexer<id>:DISPlay[:STATe]?

**Return Type** Boolean

**Overlapped?** No

**Default** OFF (0)

**SENSe<cnum>:MULTiplexer<id>:TSET9:OUTPut[:DATA] <data>**

(Read-Write) Sets the control lines of the specified E5091A. Control lines, provided through a E5091A front panel connector, are used to control external equipment such as a part handler. See your E5091A documentation to learn more about control lines.

**Parameters**

- <cnum> Channel number of the measurement. If unspecified, value is set to 1.
- <id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)
- <data> Data value used to set control lines. Values are obtained by adding weights from the following table that correspond to individual lines. HIGH =1; LOW=0.

| Line | Weight |
|------|--------|
| 1    | 1      |
| 2    | 2      |
| 3    | 4      |
| 4    | 8      |
| 5    | 16     |
| 6    | 32     |
| 7    | 64     |

|   |     |
|---|-----|
| 8 | 128 |
|---|-----|

0 - Sets all lines low

255 - Sets all lines high

**Examples** 'The following sets line 3 and 4 high. All other lines low.  
**SENS:MULT1:TSET9:OUTP 12**

**Query Syntax** SENSE<cnum>:MULTiplexer<id>:TSET9:OUTPut[:DATA]?

**Return Type** Numeric

**Overlapped?** No

**Default** 0

### SENSe<cnum>:MULTiplexer<id>:TSET9:PORT1 <char>

(Read-Write) Switches Port 1 of the specified E5091A to one of the available outputs.

#### Parameters

<cnum> Any existing channel number; if unspecified, value is set to 1.

<id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)

<char> Output port to be switched to. Choose from:

**A**

**T1** - (If Port 2 already is connected to T1, then Port 2 will be switched to T2.)

**Examples** **SENS:MULT1:TSET9:PORT1 A**

**Query Syntax** SENSE<cnum>:MULTiplexer<id>:TSET9:PORT1?

**Return Type** Character

**Overlapped?** No

**Default** A

### SENSe<cnum>:MULTiplexer<id>:TSET9:PORT2 <char>

(Read-Write) Switches Port 2 of the specified E5091A to one of the available outputs.

**Parameters**

- <num> Any existing channel number; if unspecified, value is set to 1.
- <id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)
- <char> Output port to be switched to. Choose from:  
**T1** - If Port 1 already is connected to T1, then Port 1 will be switched to A.  
**T2**

**Examples** `SENS:MULT1:TSET9:PORT2 T2`

**Query Syntax** `SENSe<num>:MULTiplexer<id>:TSET9:PORT2?`

**Return Type** Character

**Overlapped?** No

**Default** T1

---

**SENSe<num>:MULTiplexer<id>:TSET9:PORT3 <char>**

(Read-Write) Switches Port 3 of the specified E5091A to one of the available outputs.

**Parameters**

- <num> Any existing channel number; if unspecified, value is set to 1.
- <id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)
- <char> Output port to be switched to. Choose from:  
**R1** (R1+)  
**R2** (R2+)  
**R3** (R3+) If option 007 (7port), R2 is selected.

**Examples** `SENS:MULT1:TSET9:PORT3 R2`

**Query Syntax** `SENSe<num>:MULTiplexer<id>:TSET9:PORT3?`

**Return Type** Character

**Overlapped?** No

**Default** R1

---

**SENSe<num>:MULTiplexer<id>:TSET9:PORT4 <char>**

(Read-Write) Switches Port 4 of the specified E5091A to one of the available outputs.

#### Parameters

- <num> Any existing channel number; if unspecified, value is set to 1.
- <id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)
- <char> Output port to be switched to. Choose from:  
**R1** (R1-)  
**R2** (R2-)  
**R3** (R3-) If option 007 (7port), R2 is selected.

**Examples** `SENS:MULT1:TSET9:PORT4 R2`

**Query Syntax** `SENSe<num>:MULTiplexer<id>:TSET9:PORT4?`

**Return Type** Character

**Overlapped?** No

**Default** R1

---

### **SENSe:MULTiplexer<id>:STATe <bool>**

(Read-Write) Turns ON/OFF the port switching and control line output of the specified E5091A. This setting affects all channels in use by the specified testset.

If the specified testset is not connected to USB or not ON, then setting State ON will report an error. All other properties of the object can be set when the testset is not connected.

#### Parameters

- <id> Id of the E5091A test set. Choose from 1 or 2. [Learn how to set ID value.](#)
- <bool> ON(1) Turns switching ON.  
OFF (0) Turns switching OFF.

**Examples** `SENS:MULT1:STAT 1`  
`sense2:multiplexer2:state on`

**Query Syntax** `SENSe<num>:MULTiplexer<id>:STATe?`

**Return Type** Boolean

**Overlapped?** No

**Default** OFF (0)

---