

User's Guide

Agilent Technologies N5181A/82A/83A MXG Signal Generators

This guide applies to the following signal generator models:

N5181A MXG RF Analog Signal Generator

N5182A MXG RF Vector Signal Generator

N5183A MXG Microwave Analog Signal Generator

Because of our continuing efforts to improve our products through firmware and hardware revisions, signal generator design and operation may vary from descriptions in this guide. We recommend that you use the latest revision of this guide to ensure that you have up-to-date product information. Compare the print date of this guide (see bottom of page) with the latest revision, which can be downloaded from the following website:

<http://www.agilent.com/find/mxg>



Agilent Technologies

Manufacturing Part Number: N5180-90003

Printed in USA

December 2007

© Copyright 2006, 2007 Agilent Technologies, Inc.

Notice

The material contained in this document is provided “as is”, and is subject to being changed, without notice, in future editions.

Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied with regard to this manual and to any of the Agilent products to which it pertains, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or any of the Agilent products to which it pertains. Should Agilent have a written contract with the User and should any of the contract terms conflict with these terms, the contract terms shall control.

1 Signal Generator Overview

Signal Generator Features	2
Modes of Operation	3
Continuous Wave	3
Swept Signal	3
Analog Modulation	3
Digital Modulation (N5182A with Options 651, 652, or 654 Only)	3
Front Panel Overview	4
1. Host USB	4
2. Display	4
3. Softkeys	4
4. Numeric Keypad	4
5. Arrows and Select.	5
6. Page Up	5
7. MENUS	5
8. Trigger	5
9. Local Cancel/(Esc)	5
10. Help	5
11. Preset and User Preset.	6
12. RF Output	6
13. RF On/Off and LED.	6
14. Mod On/Off and LED.	6
15. Page Down.	6
16. I Input (vector models only)	6
17. Q Input (vector models only).	7
18. Knob.	7
19. Incr Set	7
20. Return	7
21. More and LED	7
22. Power Switch and LEDs	7
Front Panel Display	8
1. Active Function Area.	8
2. Frequency Area	8
3. Annunciators	9
4. Amplitude Area	10
5. Error Message Area.	10
6. Text Area	10
7. Softkey Label Area	10
Rear Panel Overview.	11
1. AC Power Receptacle	11
2. SWEEP OUT	12

Contents

3. AM	12
4. FM	12
5. PULSE	12
6. TRIG IN	12
7. TRIG OUT	12
8. REF IN	13
9. 10 MHz OUT	13
10. GPIB	13
11. LAN	13
12. Device USB	13
Digital Modulation Connectors (vector models only)	14
I OUT, Q OUT, OUT, OUT	14
EXT CLK	14
EVENT 1	14
PAT TRIG	15
DIGITAL BUS I/O	15
AUX I/O	15
2 Setting Preferences & Enabling Options	
User Preferences	18
Display Settings	18
Power On and Preset	19
Front Panel Knob Resolution	19
Setting Time and Date	20
Upgrading Firmware	20
Remote Operation Preferences	21
GPIB Address and Remote Language	21
Configuring the LAN Interface	22
Enabling LAN Services: Browser, Sockets, and VXI-11	22
Configuring the Remote Languages	23
Enabling an Option	24
Viewing Options and Licenses	24
3 Basic Operation	
Presetting the Signal Generator	26
Viewing Key Descriptions	26
Entering and Editing Numbers and Text	27
Entering Numbers and Moving the Cursor	27
Entering Alpha Characters	27
Example: Using a Table Editor	28

Setting Frequency and Power (Amplitude)	29
Example: Configuring a 700 MHz, -20 dBm Continuous Wave Output.	29
Using an External Reference Oscillator.	30
Configuring a Swept Output.	31
Routing Signals	32
Step Sweep	33
List Sweep	38
Example: Using a Single Sweep.	41
Example: Manual Control of Sweep	42
Modulating the Carrier Signal.	43
Example	43
Simultaneous Modulation	44
Working with Files	45
File Softkeys	46
Viewing a List of Stored Files.	47
Storing a File	48
Loading (Recalling) a Stored File.	49
Moving a File from One Media to Another	50
Working with Instrument State Files	51
Selecting the Default Storage Media.	55
Reading Error Messages	56
Error Message Format.	56
4 Optimizing Performance	57
Using Flatness Correction	58
Creating a User Flatness Correction Array	60
Recalling and Applying a User Flatness Correction Array	66
Using External Leveling.	67
Option 1E1 Output Attenuator Behavior and Use	69
Configure External Leveling	70
Using Unleveled Operating Modes	73
ALC Off Mode	74
Power Search Mode.	74
Using an Output Offset, Reference, or Multiplier	75
Setting an Output Offset	75
Setting an Output Reference.	76
Setting a Frequency Multiplier	77
Using Free Run, Step Dwell, and Timer Trigger	78
Understanding Free Run, Step Dwell, and Timer Trigger Setup.	78

Contents

.....	79
Using a USB Keyboard	80
5 Using Analog Modulation (Option UNT Only)	
The Basic Procedure	82
Using an External Modulation Source	83
Removing a DC Offset	83
6 Using Pulse Modulation (Option UNU or UNW)	
Pulse Characteristics	87
The Basic Procedure	89
Example	89
7 Basic Digital Operation—No BBG Option Installed	
I/Q Modulation	92
Configuring the Front Panel Inputs	93
8 Basic Digital Operation (Option 651/652/654)	
Waveform File Basics	96
Signal Generator Memory	96
Dual ARB Player	96
Storing, Loading, and Playing a Waveform Segment	98
Loading a Waveform Segment into BBG Media	98
Storing/Renaming a Waveform Segment to Internal or USB Media	99
Playing a Waveform Segment	99
Waveform Sequences	101
Creating a Sequence	102
Viewing the Contents of a Sequence	103
Editing a Sequence	103
Playing a Sequence	104
Saving a Waveform's Settings & Parameters	105
Viewing and Modifying Header Information	107
Viewing & Editing a Header without Selecting the Waveform	109
Using Waveform Markers	110
Waveform Marker Concepts	111
Accessing Marker Utilities	115
Viewing Waveform Segment Markers	116
Clearing Marker Points from a Waveform Segment	116
Setting Marker Points in a Waveform Segment	117
Viewing a Marker Pulse	119

Using the RF Blanking Marker Function	120
Setting Marker Polarity	122
Controlling Markers in a Waveform Sequence.	123
Using the EVENT Output Signal as an Instrument Trigger	125
Triggering a Waveform	126
Trigger Type	127
Trigger Source	128
Example: Segment Advance Triggering	129
Example: Gated Triggering	130
Example: External Triggering	132
Clipping a Waveform.	133
How Power Peaks Develop	134
How Peaks Cause Spectral Regrowth	136
How Clipping Reduces Peak-to-Average Power	137
Configuring Circular Clipping	140
Configuring Rectangular Clipping.	141
Scaling a Waveform	142
How DAC Over-Range Errors Occur	144
How Scaling Eliminates DAC Over-Range Errors.	145
Setting Waveform Runtime Scaling.	146
Setting Waveform Scaling	147
Setting the Baseband Frequency Offset.	149
DAC Over-Range Conditions and Scaling.	150
I/Q Modulation	152
Using the Rear Panel I and Q Outputs	153
Configuring the Front Panel Inputs	154
I/Q Adjustments.	155
I/Q Calibration	157
Multiple Baseband Generator Synchronization	158
Understanding the Master/Slave System	160
Equipment Setup	161
Configuring the Setup	161
Making Changes to the Multiple Sync Setup and Resynchronizing the Master/Slave System	163
Waveform 5-Pack Licensing (Options 221-229).	164
Understanding Waveform 5-Pack Licensing	164
Installing an Option N5182A-22x Waveform 5-Pack.	Licensing165
Licensing a Signal Generator Waveform File	165

Contents

Waveform 5-Pack Licensing Softkeys Overview.	165
Using Waveform 5-Pack History	171
Waveform 5-Pack Warning Messages	175
9 Adding Real Time Noise to a Signal (Option 403)	
Adding Real-Time Noise to a Dual ARB Waveform.	178
Example.	180
Using Real Time I/Q Baseband AWGN.	181
10 Real-Time Phase Noise Impairments (Option 432)	
Real-Time Phase Noise Impairment.	184
The Agilent MXG Phase Noise Shape and Additive Phase Noise Impairments	185
Understanding the Phase Noise Adjustments.	187
DAC Over-Range Conditions and Scaling	188
11 Custom Digital Modulation (Option 431)	
Custom Modulation	190
Custom Arb Waveform Generator	190
Using the Arbitrary Waveform Generator	195
Using Predefined Custom TDMA Digital Modulation	195
Creating a Custom TDMA Digital Modulation State.	197
Storing a Custom TDMA Digital Modulation State	198
Recalling a Custom TDMA Digital Modulation State	200
Creating a Custom Multicarrier TDMA Digital Modulation State	201
Storing a Custom Multicarrier TDMA Digital Modulation State	203
Applying Changes to an Active Multicarrier TDMA Digital Modulation State	203
Using Finite Impulse Response (FIR) Filters.	204
Creating a User-Defined FIR Filter Using the FIR Table Editor	204
Modifying a FIR Filter Using the FIR Table Editor.	208
Loading the Default Gaussian FIR File.	209
Modifying the Coefficients	210
Storing the Filter to Memory	211
12 Multitone and Two-Tone Waveform Generator (Option 430)	
Creating a Custom Two-Tone Waveform.	213
Creating a Custom Multitone Waveform	213
Using Two-Tone Modulation.	214
Two Tone Modulation Softkeys	215
Creating a Two-Tone Waveform	215

Viewing a Two-Tone Waveform	216
Minimizing Carrier Feedthrough	217
Changing the Alignment of a Two-Tone Waveform	218
Using Multitone Modulation	220
Multitone Modulation Softkeys	220
Initializing the Multitone Setup Table Editor	220
Configuring Tone Powers and Tone Phases	221
Removing a Tone	221
Generating the Waveform	221
Configuring the RF Output	222
Applying Changes to an Active Multitone Signal	222
13 Working in a Secure Environment	
Understanding Memory Types	226
Removing Data from Memory (Option 006 Only)	228
Erase All	228
Erase and Overwrite All	229
Erase and Sanitize All	229
Removing Persistent State Information Not Removed During Erase	229
Secure Mode	230
Securing a Nonfunctioning Instrument	230
Using the Secure Display (Option 006 Only)	231
14 Troubleshooting	
Display	234
The Display is Too Dark to Read	234
The Display Turns Black when Using USB Media	234
Signal Generator Lock-Up	234
RF Output	235
No RF Output	235
Power Supply Shuts Down	235
No Modulation at the RF Output	235
RF Output Power too Low	235
Distortion	235
Signal Loss While Working with a Spectrum Analyzer	236
Signal Loss While Working with a Mixer	236
Sweep	238
Cannot Turn Off Sweep	238
Sweep Appears Stalled	238
Incorrect List Sweep Dwell Time	238

Contents

List Sweep Information is Missing from a Recalled Register.	238
Amplitude Does Not Change in List or Step Sweep	238
Internal Media Data Storage	239
Instrument State Saved but the Register is Empty or Contains the Wrong State	239
USB Media Data Storage	239
Instrument Recognizes USB Media Connection, but Does Not Display Files	239
Preset	239
The Signal Generator Does Not Respond	239
Pressing Preset Performs a User Preset	239
Error Messages	240
Error Message Types	240
Error Message File	240
Front Panel Tests	241
Self Test	241
Licenses	242
A Time-Based License Quits Working	242
Cannot Load a Time-Based License	242
Contacting Agilent Technologies	243
Returning a Signal Generator to Agilent	243

Documentation Overview

- | | |
|-----------------------------|---|
| Installation Guide | <ul style="list-style-type: none">• Safety Information• Receiving the Instrument• Environmental & Electrical Requirements• Basic Setup• Accessories• Operation Verification• Regulatory Information |
| User's Guide | <ul style="list-style-type: none">• Instrument Overview• Front Panel Operation• Security• Basic Troubleshooting |
| Programming Guide | <ul style="list-style-type: none">• Remote Operation• Status Registers• Creating & Downloading Files |
| SCPI Reference | <ul style="list-style-type: none">• SCPI Basics• Command Descriptions• Programming Command Compatibility |
| Service Guide | <ul style="list-style-type: none">• Troubleshooting• Assembly Replacement• Replaceable Parts• Post-Repair Procedures• Safety and Regulatory Information |
| Key Help^a | <ul style="list-style-type: none">• Key function description• Related SCPI commands |

^aPress the **Help** hardkey, and then the key for which you wish help.

1 Signal Generator Overview

- [Signal Generator Features](#) on page 2
- [Modes of Operation](#) on page 3
- [Front Panel Overview](#) on page 4
- [Front Panel Display](#) on page 8
- [Rear Panel Overview](#) on page 11

Signal Generator Features

- N5181A, RF analog models: 100 kHz to 1, 3, or 6 GHz (Options 501, 503, and 506 respectively)
N5182A, RF vector models: 100 kHz to 3 or 6 GHz (Options 503, and 506 respectively)
N5183A, Microwave analog model: 100 kHz to 20, 31.8, or 40 GHz (Options 520, 532, and 540 respectively)
- electronic attenuator (N5181A/82A Only)
- mechanical attenuator (N5183A with Option 1E1 Only)
- step & list sweep of frequency, power, or frequency and power
vector models can include waveforms in list sweep
- user flatness correction
- automatic leveling control (ALC); power calibration
- 10 MHz reference oscillator with external output
- flexible reference input, 1 – 50 MHz (Option 1ER)
- GPIB, USB 2.0, and 100Base-T LAN interfaces
- analog modulation: AM, FM, and Φ M (Option UNT)
- external AM, FM, and Φ M inputs (Option UNT)
- adjustable pulse delay (Option UNU)
- narrow pulse modulation (Option UNW)
- SCPI and IVI-COM driver
- 8648/ESG code compatible
- LXI Class C compliant
- multiple baseband generator synchronization when using multiple signal generators (master/slave setup)
- external analog I/Q inputs (vector models)
- phase noise interference (vector models, Option 432)
- analog differential I/Q outputs (vector models, Option 1EL)
- arbitrary I/Q waveform playback up to 125 MSa/s (vector models, Option 654)
- with Signal Studio Software, vector models can generate 802.11 WLAN, W-CDMA, cdma2000, 1xEV-DO, GSM, EDGE, and more

For more details on hardware, firmware, software, and documentation features and options, refer to the data sheet shipped with the signal generator and available from the Agilent Technologies website.

1. Open: <http://www.agilent.com/find/mxg>
2. Select the desired model number.
3. In the options and price list section, click **price list**.

Modes of Operation

Depending on the model and installed options, the Agilent MXG signal generator provides up to four basic modes of operation: continuous wave (CW), swept signal, analog modulation, and digital modulation.

Continuous Wave

In this mode, the signal generator produces a continuous wave signal. The signal generator is set to a single frequency and power level. Both the N5182A and N5181A can produce a CW signal.

Swept Signal

In this mode, the signal generator sweeps over a range of frequencies and/or power levels. Both the N5182A and N5181A provide list and step sweep functionality.

Analog Modulation

In this mode, the signal generator modulates a CW signal with an analog signal. The analog modulation types available depend on the installed options.

Option UNT provides AM, FM, and Φ M modulations. Some of these modulations can be used together.

Options UNU and UNW provide standard and narrow pulse modulation capability, respectively.

Digital Modulation (N5182A with Options 651, 652, or 654 Only)


NOTE The internal baseband generator speed upgrade Options 670, 671, and 672 are option upgrades that *require* Option 651 and 652 to have been loaded at the factory (refer to the *Data Sheet* for more information). Any references to 651, 652, or 654 are inclusive of 671, 672, and 674.

In this mode, the signal generator modulates a CW signal with an arbitrary I/Q waveform. I/Q modulation is only available on the N5182A. An internal baseband generator (Option 651, 652, or 654) adds the following digital modulation formats:

- *Custom Arb Waveform Generator* mode can produce a single-modulated carrier or multiple-modulated carriers. Each modulated carrier waveform must be calculated and generated before it can be output; this signal generation occurs on the internal baseband generator. Once a waveform has been created, it can be stored and recalled, which enables repeatable playback of test signals. To learn more, refer to [“Using the Arbitrary Waveform Generator” on page 195](#).
- *Multitone* mode produces up to 64 continuous wave signals (or tones). Like the Two Tone mode, the frequency spacing between the signals and the amplitudes are adjustable. To learn more, refer to [“Creating a Custom Multitone Waveform” on page 213](#).
- *Two-tone* mode produces two separate continuous wave signals (or tones). The frequency spacing between the signals and the amplitudes are adjustable. To learn more, refer to [“Creating a Custom Two-Tone Waveform” on page 213](#).
- *Dual ARB* mode is used to control the playback sequence of waveform segments that have been written into the ARB memory located on the internal baseband generator. These waveforms can be generated by the internal baseband generator using the Custom Arb Waveform Generator

mode, or downloaded through a remote interface into the ARB memory. To learn more, refer to “Dual ARB Player” on page 96.

Front Panel Overview

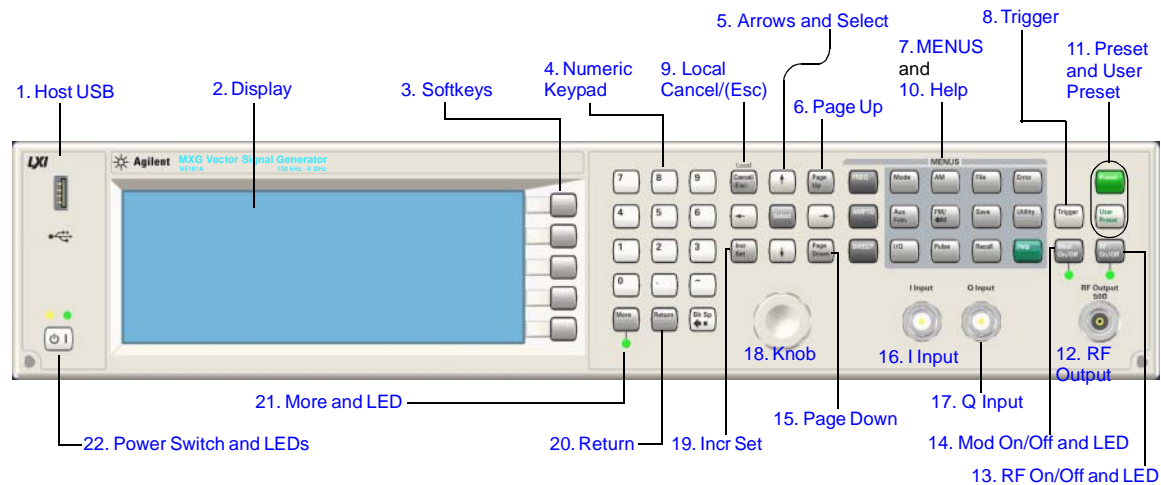

1. Host USB

Connector Type A

USB Protocol 2.0

Use this universal serial bus (USB) to connect a memory stick for data transfer. You can connect or disconnect a USB device without shutting down or restarting the signal generator. The instrument also has a rear-panel device USB connector (see [page 13](#)) used to remotely control the instrument.

2. Display

The LCD screen provides information on the current function. Information can include status indicators, frequency and amplitude settings, and error messages. Labels for the softkeys are located on the right-hand side of the display. See also, “[Front Panel Display](#)” on [page 8](#).

3. Softkeys

A softkey activates the function indicated by the displayed label to the left of the key.

4. Numeric Keypad

The numeric keypad comprises the 0 through 9 hardkeys, a decimal point hardkey, a minus sign hardkey, and a backspace hardkey. See “[Entering and Editing Numbers and Text](#)” on [page 27](#).

5. Arrows and Select


The **Select** and arrow hardkeys enable you to select items on the signal generator’s display for editing. See [“Entering and Editing Numbers and Text” on page 27](#).

6. Page Up

In a table editor, use this hardkey to display a previous page. See [“Example: Using a Table Editor” on page 28](#). When text does not fit on one page in the display area, use this key in conjunction with the [Page Down](#) key ([page 6](#)) to scroll text.

7. MENUS

These hardkeys open softkey menus that enable you to configure instrument functions or access information.

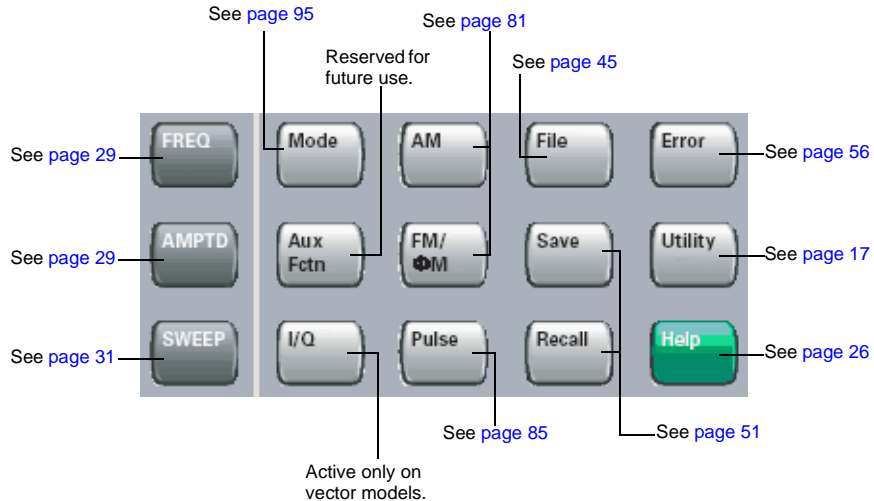

8. Trigger

When trigger mode is set to **Trigger Key**, this hardkey initiates an immediate trigger event for a function such as a list or step sweep.

9. Local Cancel/(Esc)

This hardkey deactivates remote operation and returns the signal generator to front panel control, cancels an active function entry, and cancels long operations (such as an IQ calibration).

10. Help

Use this key to display a description of any hardkey or softkey. See [“Viewing Key Descriptions” on page 26](#).

11. Preset and User Preset

These hardkeys set the signal generator to a known state (factory or user-defined). See [“Presetting the Signal Generator”](#) on page 26.

12. RF Output

Connector Standard: female Type-N
 Option 1EM: Rear panel female Type-N
 Impedance: 50Ω

Damage Levels 50Vdc, 2W maximum RF power

13. RF On/Off and LED

This hardkey toggles the operating state of the RF signal present at the RF OUTPUT connector. The RF On/Off LED lights when RF output is enabled.

14. Mod On/Off and LED

This hardkey enables or disables the modulation of the output carrier signal by an active modulation format. This hardkey does not set up or activate a format (see [“Modulating the Carrier Signal”](#) on page 43).

The MOD ON/OFF LED lights when modulation of the output is enabled.

15. Page Down

In a table editor, use this hardkey to display the next page. See [“Example: Using a Table Editor”](#) on page 28. When text does not fit on one page in the display area, use this key in conjunction with the [Page Up](#) key (page 5) to scroll text.

16. I Input (vector models only)

Connector Type: female BNC Impedance: 50Ω

Signal An externally supplied analog, in-phase component of I/Q modulation.

The signal level is $\sqrt{I^2+Q^2} = 0.5 V_{\text{rms}}$ for a calibrated output level.

Damage Levels 1V_{rms}

See also, [“I/Q Modulation”](#) on page 152.

17. Q Input (vector models only)

Connector Type: female BNC Impedance: 50Ω

Signal An externally supplied analog, quadrature-phase component of I/Q modulation.

The signal level is $\sqrt{I^2+Q^2} = 0.5 V_{\text{rms}}$ for a calibrated output level.

Damage Levels $1V_{\text{rms}}$

See also, [“I/Q Modulation” on page 152.](#)

18. Knob

Rotating the knob increases or decreases a numeric value, or moves the highlight to the next digit, character, or item in a list. See also, [“Front Panel Knob Resolution” on page 19.](#)

19. Incr Set

This hardkey enables you to set the increment value of the currently active function. The increment value also affects how much each turn of the knob changes an active function’s value, according to the knob’s current ratio setting (see [“Front Panel Knob Resolution” on page 19.](#))

20. Return

This hardkey enables you to retrace key presses. In a menu with more than one level, the **Return** key returns to the prior menu page.


21. More and LED

When a menu contains more softkey labels than can be displayed, the More LED lights and a More message displays below the labels. To display the next group of labels, press the **More** hardkey.

22. Power Switch and LEDs

This switch selects the standby mode or the power on mode. In the standby position, the yellow LED lights and all signal generator functions deactivate. The signal generator remains connected to the line power, and some power is consumed by some internal circuits. In the on position, the green LED lights and the signal generator functions activate.

Front Panel Display

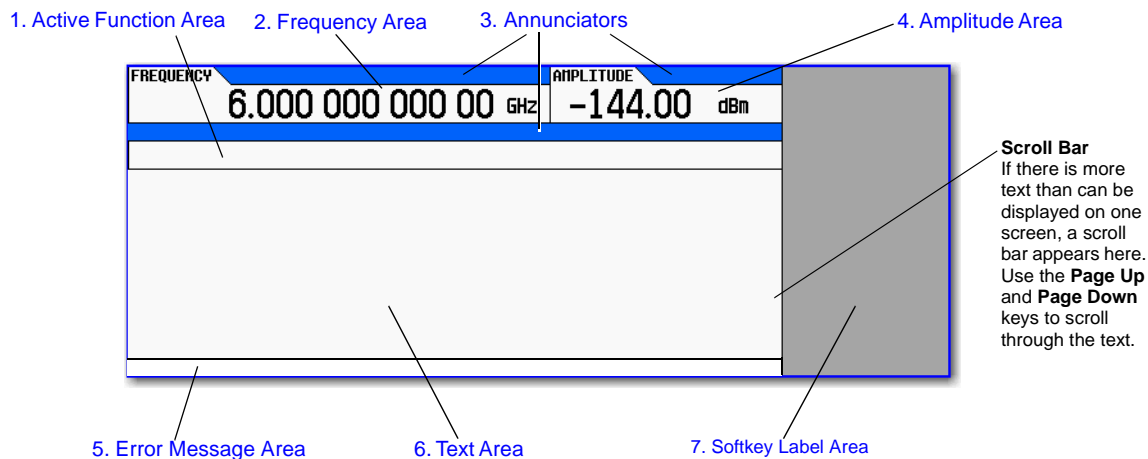

1. Active Function Area

This area displays the currently active function. For example, if frequency is the active function, the current frequency setting appears. If the currently active function has an increment value associated with it, that value also appears.

2. Frequency Area

This area displays the current frequency setting.

3. Annunciators

Annunciators show the status of some of the signal generator functions, and indicate error conditions. An annunciator position may be used by more than one annunciator; in this case, only one of the functions sharing a given position can be active at a given time.

This annunciator appears when...

ΦM	Phase modulation is on. If you turn frequency modulation on, the FM annunciator replaces ΦM.
ARB	The ARB generator is on.
ALC OFF	The ALC circuit is disabled. The UNLEVEL annunciator appears in the same position if the ALC is enabled and is unable to maintain the output level.
AM	Amplitude modulation is on.
ARMED	A sweep has been initiated and the signal generator is waiting for the sweep trigger event.
ATTNHOLD	The attenuator hold function is on. When this function is on, the attenuator is held at its current setting.
BEG DAC	A DAC overflow is occurring, adjust the runtime scaling adjust until the BEG DAC annunciator turns off. Another annunciator, UNLOCK, appears in the same position and has priority over the BEG DAC annunciator (see UNLOCK, below).
DETHTR	The ALC detector heater is not up to temperature. To meet ALC specifications the heater must be at temperature.
AWGN	Real Time I/Q Baseband additive white Gaussian noise is on.
DIGBUS	The digital bus is in use.
DIGMOD	Custom Arb waveform generator is on.
ERR	An error message is placed in the error queue. This annunciator does not turn off until you either view all of the error messages or clear the error queue (see “Reading Error Messages” on page 56).
EXTREF	An external frequency reference is applied.
FM	Frequency modulation is on. If you turn phase modulation on, the ΦM annunciator replaces FM.
I/Q	I/Q vector modulation is on.
L	The signal generator is in listener mode and is receiving information or commands over the GPIB, USB, or VXI-11/Sockets (LAN) interface.
M-TONE	Multitone waveform generator is on.
MULT	A frequency multiplier is set (see “Setting a Frequency Multiplier” on page 77).
OFFS	An output offset is set (see “Setting an Output Offset” on page 75).
PN	Phase noise interference is on.
PULSE	Pulse modulation is on.
R	The signal generator is remotely controlled over the GPIB, USB, or VXI-11/Sockets (LAN) interface. When the signal generator is in remote mode, the keypad is locked out. To unlock the keypad, press Local .
REF	An output reference is set (see “Setting an Output Reference” on page 76).
RF OFF	The signal generator’s RF Output is not enabled.
S	The signal generator has generated a service request (SRQ) over the GPIB, USB, or VXI-11/Sockets (LAN) interface.
SWEEP	The signal generator is currently sweeping in list or step mode.
SWMAN	The signal generator is in manual sweep mode.
T	The signal generator is in talker mode and is transmitting information over the GPIB, USB, or VXI-11/Sockets (LAN) interface.
T-TONE	Two-Tone waveform generator is on.

This annunciator appears when...

UNLEVEL	The signal generator is unable to maintain the correct output level. This is not necessarily an indication of instrument failure; unlevelled conditions can occur during normal operation. Another annunciator, ALC OFF, appears in the same position when the ALC circuit is disabled (see ALC OFF, above).
UNLOCK	Any of the phase locked loops cannot maintain phase lock. To determine which loop is unlocked, examine the error messages (see “Reading Error Messages” on page 56).
WINIT	The signal generator is waiting for you to initiate a single sweep.

4. Amplitude Area

This area displays the current output power level setting (If the RF Output is off, this area is greyed out).

5. Error Message Area

This area displays abbreviated error messages. If multiple messages occur, only the most recent message remains displayed. See [“Reading Error Messages” on page 56](#).

6. Text Area

This area displays signal generator status information, such as the modulation status, and other information such as sweep lists and file catalogs. This area also enables you to perform functions such as managing information (entering information, and displaying or deleting files).


7. Softkey Label Area

This area displays labels that define the function of the softkeys located immediately to the right of the display. Softkey labels change, depending on the function selected.

Rear Panel Overview

Digital Modulation Connectors (vector models only) on page 14

1. AC Power Receptacle

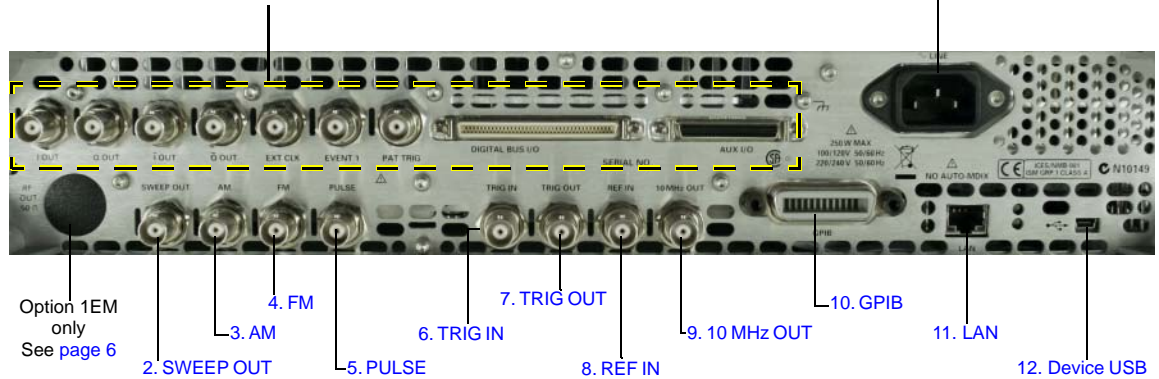

1. AC Power Receptacle

The AC power cord receptacle accepts a three-pronged AC power cord that is supplied with the signal generator. For details on line setting requirements and the power cord, see the *Installation Guide*.

2. SWEEP OUT

Connector female BNC Impedance $<1\Omega$
Can drive 2 k Ω .

Signal Voltage range: 0 to +10V, regardless of sweep width
In swept mode: beginning of sweep = 0V; end of sweep = +10V
In CW mode: no output

This is a multiple use connector. For signal routing selections, see pages [32](#) and [85](#).

3. AM

Connector female BNC Impedance nominally 50 Ω

Signal An externally supplied $\pm 1V_p$ signal that produces the indicated depth.

Damage Levels 5V_{rms} and 10V_p

4. FM

Connector female BNC Impedance nominally 50 Ω

Signal An externally supplied $\pm 1V_p$ signal that produces the indicated deviation

Damage Levels 5V_{rms} and 10V_p

5. PULSE

Connector female BNC Impedance nominally 50 Ω

Signal Externally supplied: +1V = on; 0V = off

Damage Levels 5V_{rms} and 10V_p

6. TRIG IN

Connector female BNC Impedance high Z

Signal An externally supplied TTL or CMOS signal for triggering operations, such as point-to-point in manual sweep mode or an LF sweep in external sweep mode. Triggering can occur on either the positive or negative edge.

Damage Levels $\leq -0.5V$ and $\geq +5.5V$

7. TRIG OUT

Connector female BNC Impedance nominally 50 Ω

Signal A TTL signal that is high at the start of a dwell sequence, or when waiting for the point trigger in manual sweep mode.
It is low when the dwell is over, or when the point trigger is received.
The logic polarity can be reversed.

This is a multiple use connector. For signal routing selections, see pages [32](#) and [85](#).

8. REF IN

Connector female BNC Impedance nominally 50 Ω

Signal An externally supplied -3.5 to $+20$ dBm signal from a timebase reference that is within ± 1 ppm.

In its factory default mode, the signal generator can detect a valid reference signal at this connector and automatically switch from internal to external reference operation. See “[Presetting the Signal Generator](#)” on page [26](#). With Option 1ER (flexible reference input), you must explicitly tell the signal generator the external reference frequency you wish to use; enter the information through the front panel or over the remote interface.

9. 10 MHz OUT

Connector female BNC Impedance nominally 50 Ω

Signal A nominal signal level greater than 4 dBm.

10. GPIB

This connector enables communication with compatible devices such as external controllers, and is one of three connectors available to remotely control the signal generator (see also [11. LAN](#) and [12. Device USB](#)).

11. LAN

The signal generator supports local area network (LAN) based communication through this connector, which enables a LAN-connected computer to remotely program the signal generator. The LAN interface is LXI class C compliant; it does not support auto-MDIX. The signal generator is limited to 100 meters on a single cable (100Base-T). For more information on the LAN, refer to the *Programming Guide*.

12. Device USB

Connector Mini-B

USB Protocol Version 2.0

Use this universal serial bus (USB) connector to connect a PC to remotely control the signal generator.

Digital Modulation Connectors (vector models only)

I OUT, Q OUT, \bar{I} OUT, \bar{Q} OUT

Connector Type: female BNC Impedance: 50 Ω
DC-coupled

Signal

I OUT The analog, in-phase component of I/Q modulation from the internal baseband generator.

Q OUT The analog, quadrature-phase component of I/Q modulation from the internal baseband generator.

\bar{I} OUT Used in conjunction with the I OUT connector to provide a balanced^a baseband stimulus.

\bar{Q} OUT Used in conjunction with the Q OUT connector to provide a balanced^a baseband stimulus.

Damage Levels > 1 Vrms **DC Origin Offset** typically <10 mV

Output Signal Levels into a 50 Ω Load

- 0.5V_{pk}, typical, corresponds to one unit length of the I/Q vector
- 0.69V_{pk} (2.84 dB), typical, maximum crest factor for peaks for $\pi/4$ DQPSK, alpha = 0.5
- 0.71V_{pk} (3.08 dB), typical, maximum crest factor for peaks for $\pi/4$ DQPSK, alpha = 0.35
- Typically 1V_{p-p} maximum

^aBalanced signals are signals present in two separate conductors that are symmetrical relative to ground, and are opposite in polarity (180 degrees out of phase).

EXT CLK

Connector female BNC Impedance nominally 50 Ω

Signal An externally supplied TTL or CMOS bit clock signal where the rising edge aligns with the beginning data bit.

The falling edge is used to clock external signals.

This signal is used with digital modulation applications.

Damage Levels > +8 and < -4V **Maximum Clock Rate** 50 MHz

EVENT 1

Connector female BNC Impedance: nominally 50 Ω

Signal A pulse that can be used to trigger the start of a data pattern, frame, or timeslot. Adjustable to \pm one timeslot; resolution = one bit

Markers

Each Arb-based waveform point has a marker on/off condition associated with it.

Marker 1 level = +3.3V CMOS high (positive polarity selected); -3.3V CMOS low (negative polarity selected).

Output on this connector occurs whenever Marker 1 is on in an Arb-based waveform (see [“Using Waveform Markers” on page 110](#)).

Damage Levels >+8 and <-4V

PAT TRIG

Connector female BNC Impedance: nominally 50Ω

Signal A TTL/CMOS low to TTL/CMOS high, or TTL/CMOS high to TTL/CMOS low edge trigger. The input to this connector triggers the internal digital modulation pattern generator to start a single pattern output or to stop and re-synchronize a pattern that is being continuously output. To synchronize the trigger with the data bit clock, the trigger edge is latched, then sampled during the falling edge of the internal data bit clock. This is the external trigger for all ARB waveform generator triggers.

Minimum Trigger Input Pulse Width (high or low) = 100 ns

Minimum Trigger Delay (trigger edge to first bit of frame) = 1.5 to 2.5 bit clock periods

Damage Levels > +8 and < -4V

DIGITAL BUS I/O

This is a proprietary bus used by Agilent Technologies signal creation software. This connector is not operational for general purpose use. Signals are present only when a signal creation software option is installed (for details, refer to <http://www.agilent.com/find/signalcreation>).

AUX I/O



The AUX I/O connector is a shielded .050 series board mount connector.

Pin 1 = Event 1
Pin 2 = Event 2
Pin 3 = Event 3
Pin 4 = Event 4
Pin 5 = Sample Rate Clock Out
Pin 6 = Patt Trig 2

Pins 7–25 = Reserved*

Pins 26–50 = Ground

*Future Capability

Event 1, 2, 3, and 4 (pins 1 – 4)

A pulse that can be used to trigger the start of a data pattern, frame, or timeslot. Adjustable to \pm one timeslot; resolution = one bit

Markers

Each Arb-based waveform point has a marker on/off condition associated with it.

Marker level = +3.3V CMOS high (positive polarity selected); -3.3V CMOS low (negative polarity selected).

Sample Rate Clock Out (pin 5)

This output is used with an internal baseband generator. This pin relays a CMOS bit clock signal for synchronizing serial data. Damage levels: > +5.5 and < -0.5V.

Patt Trig 2 (pin 6)

A TTL/CMOS low to TTL/CMOS high, or TTL/CMOS high to TTL/CMOS low edge trigger.


The input to this connector triggers the internal digital modulation pattern generator to start a single pattern output or to stop and re-synchronize a pattern that is being continuously output.

To synchronize the trigger with the data bit clock, the trigger edge is latched, then sampled during the falling edge of the internal data bit clock.

This is an external trigger for all ARB waveform generator triggers. Minimum pulse width = 100 ns. Damage levels: > +5.5 and < -0.5V.

2 Setting Preferences & Enabling Options

The Utility menu provides access to both user and remote operation preferences, and to the menus in which you can enable instrument options.

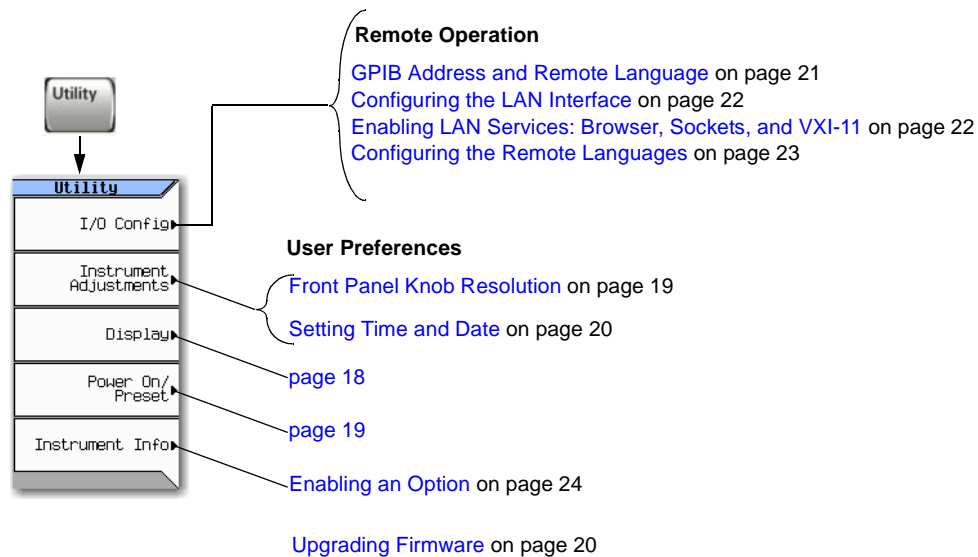

User Preferences


From the Utility menu, you can set the following user preferences:

- [Display Settings](#), below
- [Power On and Preset](#) on page 19
- [Front Panel Knob Resolution](#) on page 19

Display Settings

See also, [Using the Secure Display \(Option 006 Only\)](#) on page


Utility > Display

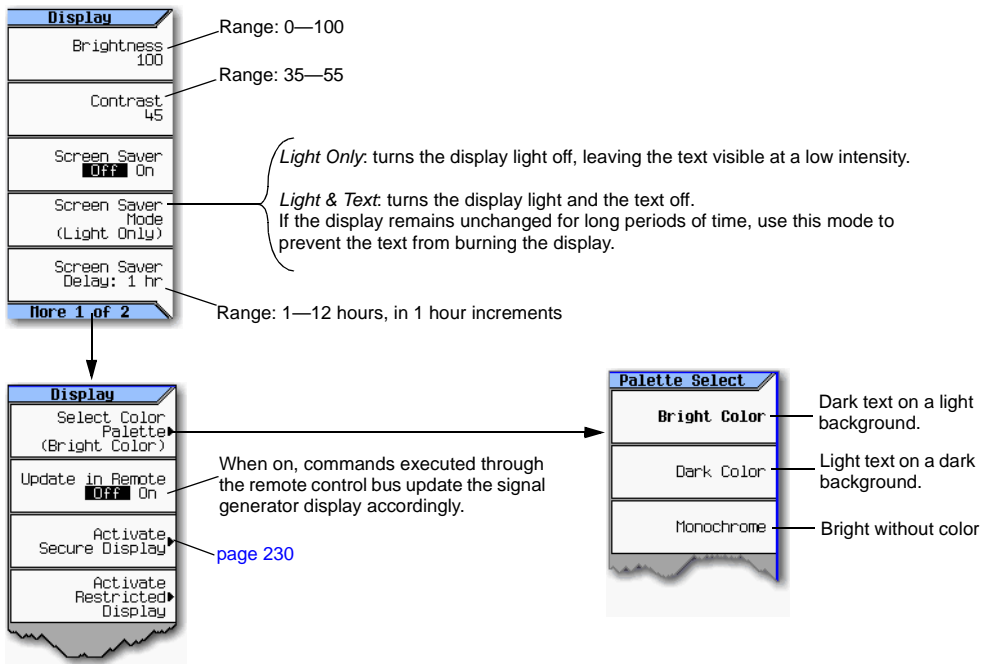

For details on each key, use key help

NOTE With both brightness and contrast set to minimum, the display may be too dark to see the softkeys. If this happens, use the figure above to locate the brightness and contrast softkeys and adjust their values so that you can see the display.

Power On and Preset

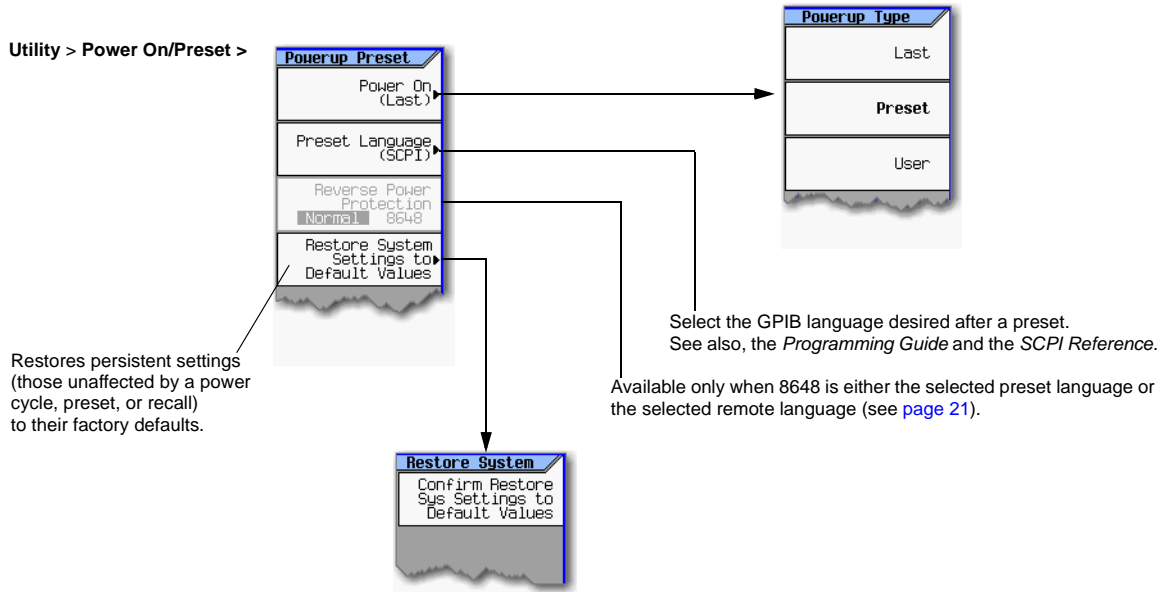

Note

To define a user preset, set the instrument up as desired and press **User Preset > Save User Preset**.

Front Panel Knob Resolution



— Makes the increment value of the current function the active entry.

Utility >
Instrument Adjustments >



The increment value and the step/knob ratio determine how much each turn of the knob changes the active function value.

For example, if the increment value of the active function is 10 dB and the step/knob ratio is 50 to 1, each turn of the knob changes the active function by 0.2 dB (1/50th of 10 dB).

To change the amount for each turn of the knob, modify the increment value, the step/knob ratio, or both.


For details on each key, use key help as described on [page 26](#).

Setting Time and Date

CAUTION Changing the time or date can adversely affect the signal generator's ability to use time-based licenses, even if a time-based license is not installed.


The signal generator's firmware tracks the time and date, and uses the *latest* time and date as its time/date reference point.

Utility >
Instrument Adjustments >

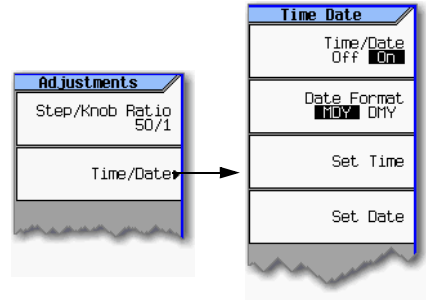

Setting the Time or Date Forward

If you set the time or date forward, be aware that you are using up any installed time-based licenses, and that you are *resetting the signal generator's time/date reference point*. When you set a new time or date that is later than the signal generator's current reference point, that date becomes the new reference point. If you then set the date back, you run the risk described in the next section.



Setting the Time or Date Backward

When you set the time back, the signal generator notes that the time has moved back from the reference point. If you set the time back more a few hours, you disable the signal generator's ability to use time-based licenses, even if there is no license installed at the time that you set the time back. In this case, you can reenable the signal generator's ability to use time-based licenses by moving the clock forward to the original time or simply waiting that length of time.


Upgrading Firmware

For information on new firmware releases, go to <http://www.agilent.com/find/upgradeassistant>.

Remote Operation Preferences

For details on operating the signal generator remotely, refer to the *Programming Guide*.

GPIO Address and Remote Language

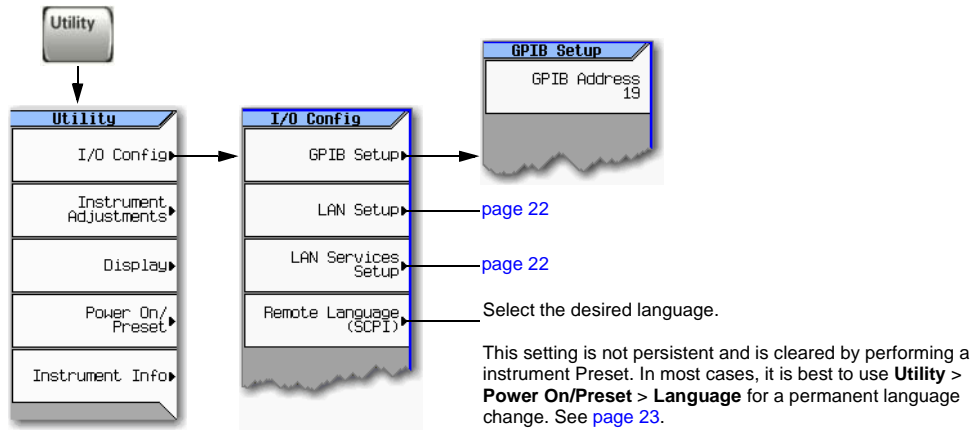


NOTES

USB is also available. It is not shown in the menu because it requires no configuration.


For details on using the instrument remotely, see the *Programming Guide*.

For details on each key, use key help as described on page 26.

Configuring the LAN Interface

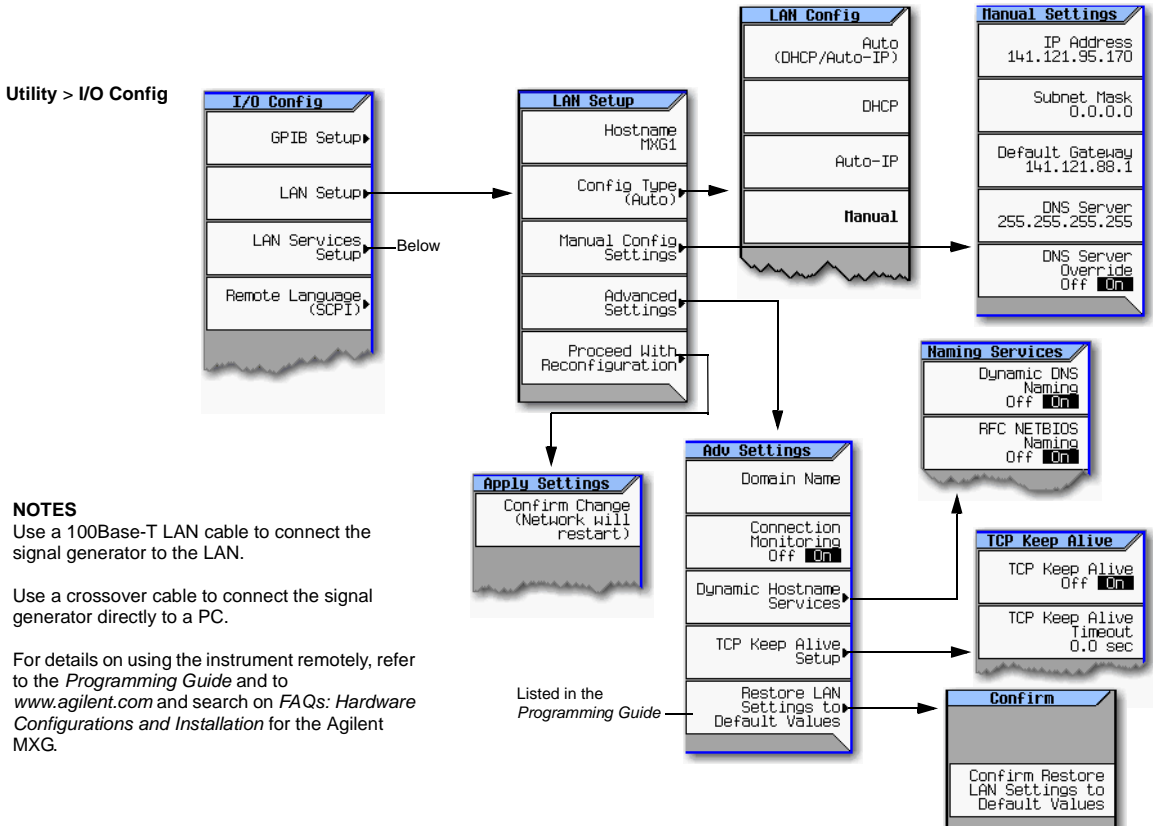

Enabling LAN Services: Browser, Sockets, and VXI-11

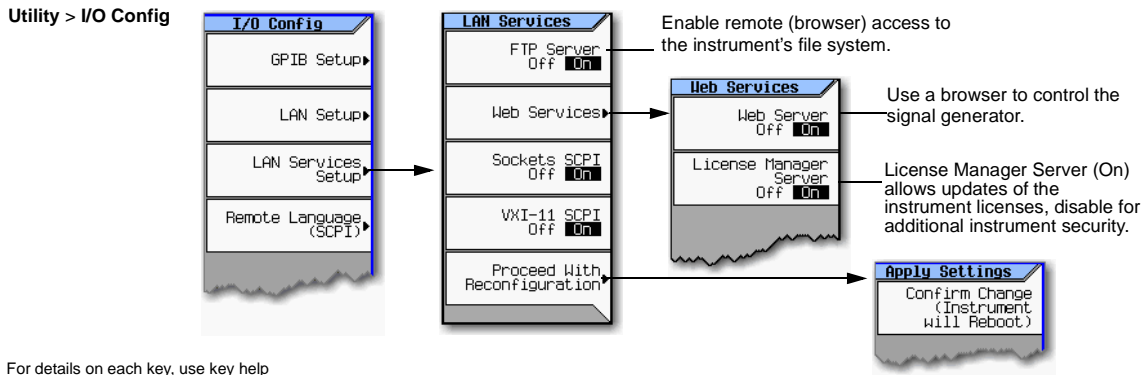

For details on each key, use key help as described on [page 26](#).

Configuring the Remote Languages

Figure 2-1 N5181A/82A

Utility > I/O Config >


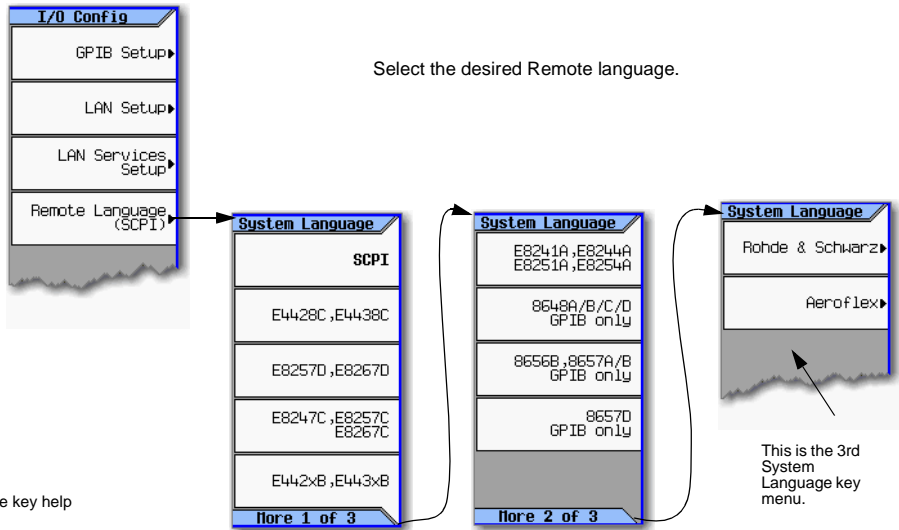


Figure 2-2 N5183A

Utility > I/O Config >

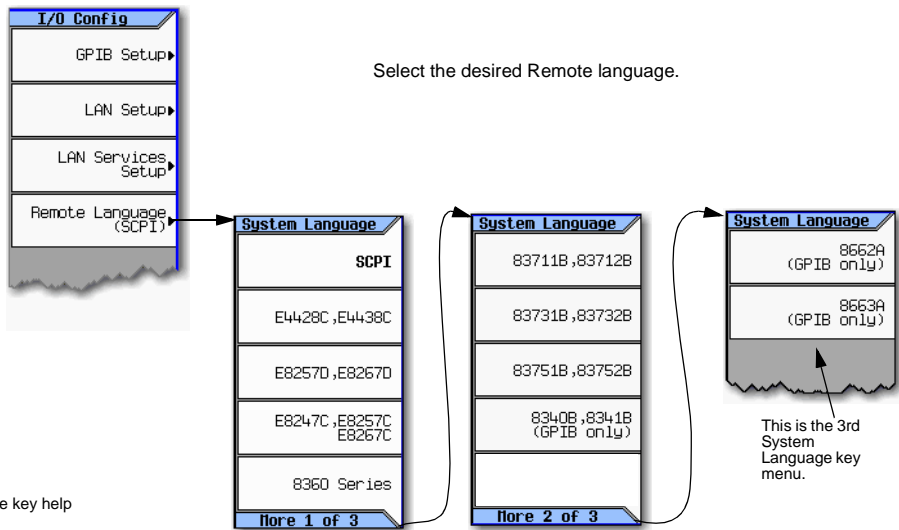


Enabling an Option

There are two ways to enable an option:

- Use the License Manager software utility:
 1. Run the utility and follow the prompts.
 2. Download the utility from www.agilent.com/find/LicenseManager and select license (.lic) files from an external USB memory drive.
- Use SCPI commands, as described in the *Programming Guide*.

Viewing Options and Licenses

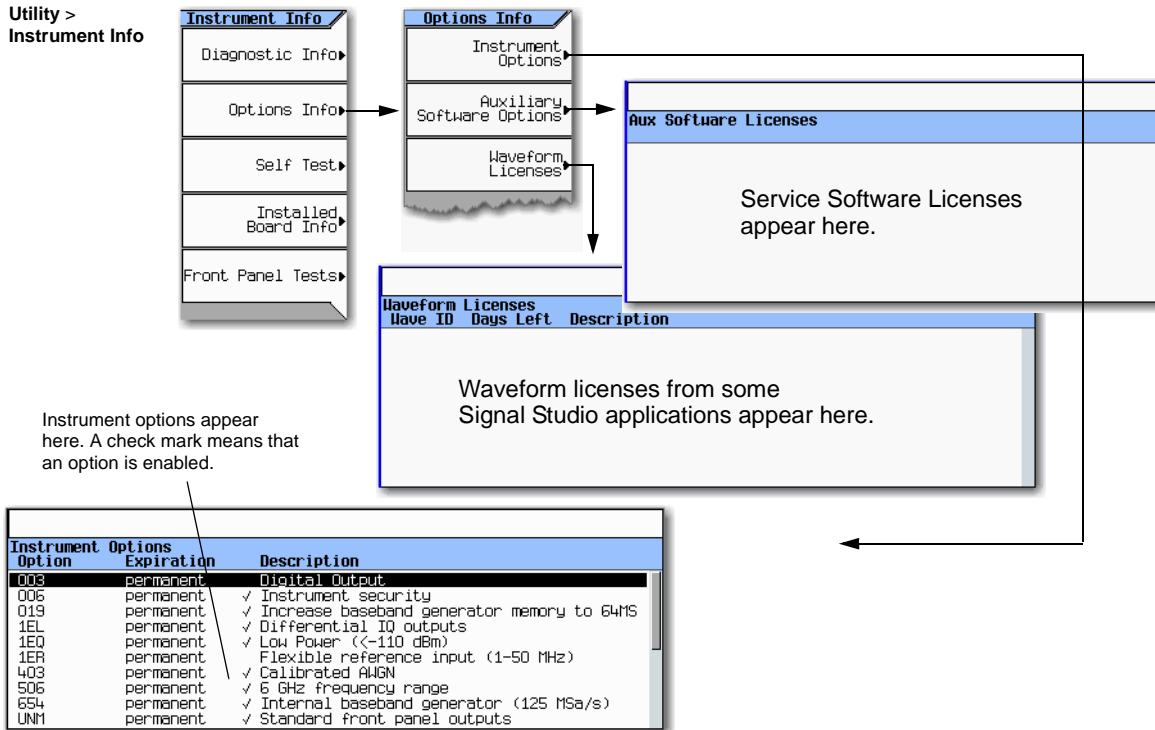

For details on each key, use key help as described on [page 26](#).

3 Basic Operation

This chapter introduces fundamental front panel operation. For information on remote operation, refer to the *Programming Guide*.

- [Presetting the Signal Generator](#) on page 26
- [Viewing Key Descriptions](#) on page 26
- [Entering and Editing Numbers and Text](#) on page 27
- [Setting Frequency and Power \(Amplitude\)](#) on page 29
- [Configuring a Swept Output](#) on page 31
- [Modulating the Carrier Signal](#) on page 43
- [Working with Files](#) on page 45
- [Reading Error Messages](#) on page 56

Presetting the Signal Generator



— To return the signal generator to a known state, press either **Preset** or **User Preset**.

Preset is the factory preset; *User Preset* is a custom preset* (see also, [page 19](#)).

To reset persistent settings (those unaffected by preset, user preset, or power cycle), press: **Utility > Power On/Presets > Restore System Defaults**.

*You can create more than one user preset by giving each saved state file a different name (see [Figure 3-10 on page 54](#)).

Viewing Key Descriptions



— The Help hardkey enables you to display a description of any hardkey or softkey.

To display help text:

1. Press **Help**.
2. Press the desired key.

The help displays and the key's normal function does not execute.

Entering and Editing Numbers and Text

Entering Numbers and Moving the Cursor

Use the number keys and decimal point to enter numeric data.

Up/down arrow keys increase/decrease a selected (highlighted) numeric value, and move the cursor vertically.

Page up/down keys move tables of data up and down within the display area.

Left/right arrow keys move the cursor horizontally.

Use the **Select** hardkey to choose part of an entry, as when entering alpha characters. In some menus, the **Select** key also acts as a terminator, and is equivalent to the **Enter** softkey.

To specify a negative value, enter the negative sign either before or after the numeric value (this key is a toggle).

Backspace moves the cursor to the left, deleting characters as it goes.



Note: Rotating the knob increases or decreases a numeric value, changes a highlighted digit or character, or steps through lists or items in a row.

See also, [Front Panel Knob Resolution](#) on page 19

For details on each key, see [page 26](#).

Entering Alpha Characters

Note: File names are limited to 25 characters.


Data entry softkeys appear in various menus. If their meaning is not clear in context, use the help key (described on [page 26](#)) to display an explanation. Use the softkey next to the alpha table for help on the table.

Selecting data that accepts alpha characters, displays one of the menus shown at right.



Use the arrow keys or knob to highlight the desired letter, then press the **Select** hardkey (or the softkey next to the alpha table). To correct errors, use **Bk Sp** or **Clear Text**.

To terminate the entry, press the **Enter** softkey.

A subset of this menu appears for hexadecimal characters. The character menu displays only the letters A through F (use the numeric keypad for other values).

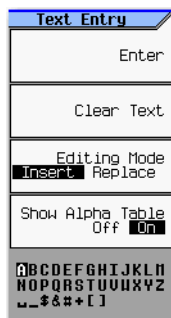

to move the cursor within the active value rather than within the alpha table, turn the alpha table off.

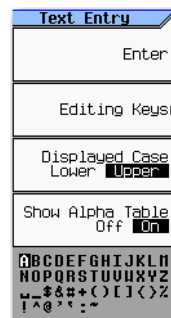


Add/edit comments for saved instrument state files (see [page 51](#)).

Example: Using a Table Editor

Table editors simplify configuration tasks. The following procedure describes basic table editor functionality using the List Mode Values table editor.

1. Preset the signal generator: Press **Preset**.
2. Open the table editor: Press **Sweep > More > Configure List Sweep**.

The signal generator displays the editor shown in the following figure.

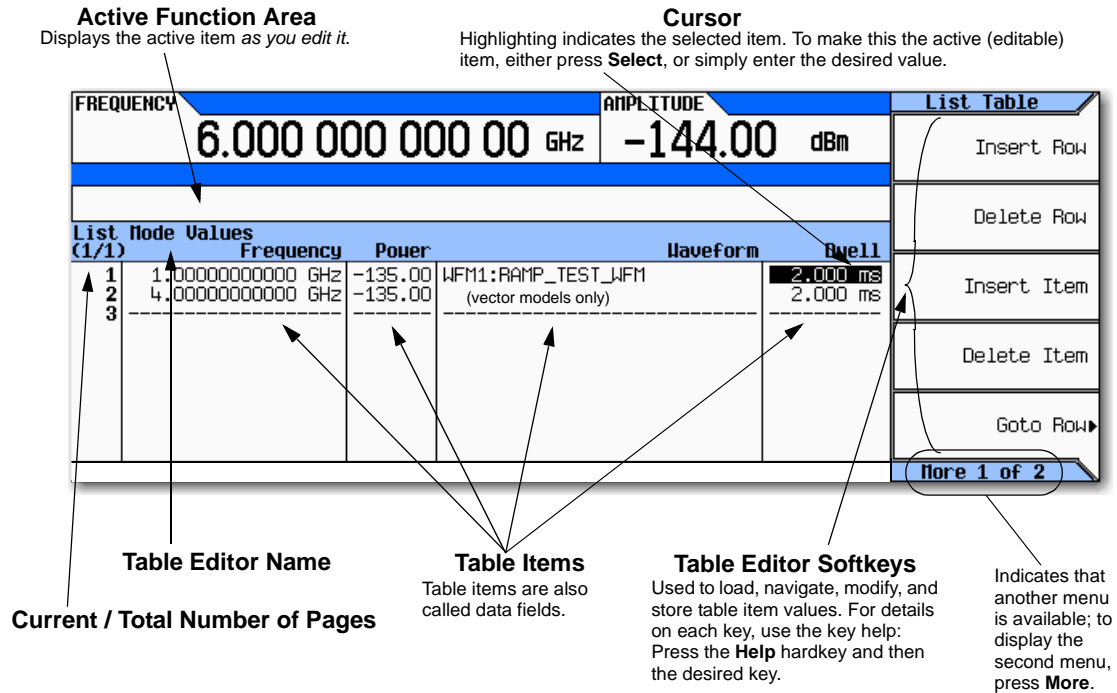


3. Highlight the desired item: use the arrow keys or the knob to move the cursor.
4. (Optional) Display the selected item in the active function area: Press **Select**.
5. Modify the value:
 - If the value is displayed in the active function area, use the knob, arrow keys, or numeric keypad to modify the value.
 - If the value is not displayed in the active function area, use the numeric keypad to enter the desired value (which then appears in the active function area).
6. Terminate the entry:
 - If available, press the desired units.
 - If units are not displayed, press either **Enter** (if available) or **Select**.

The modified item is displayed in the table.

Setting Frequency and Power (Amplitude)

Figure 3-1 Frequency and Amplitude Softkeys

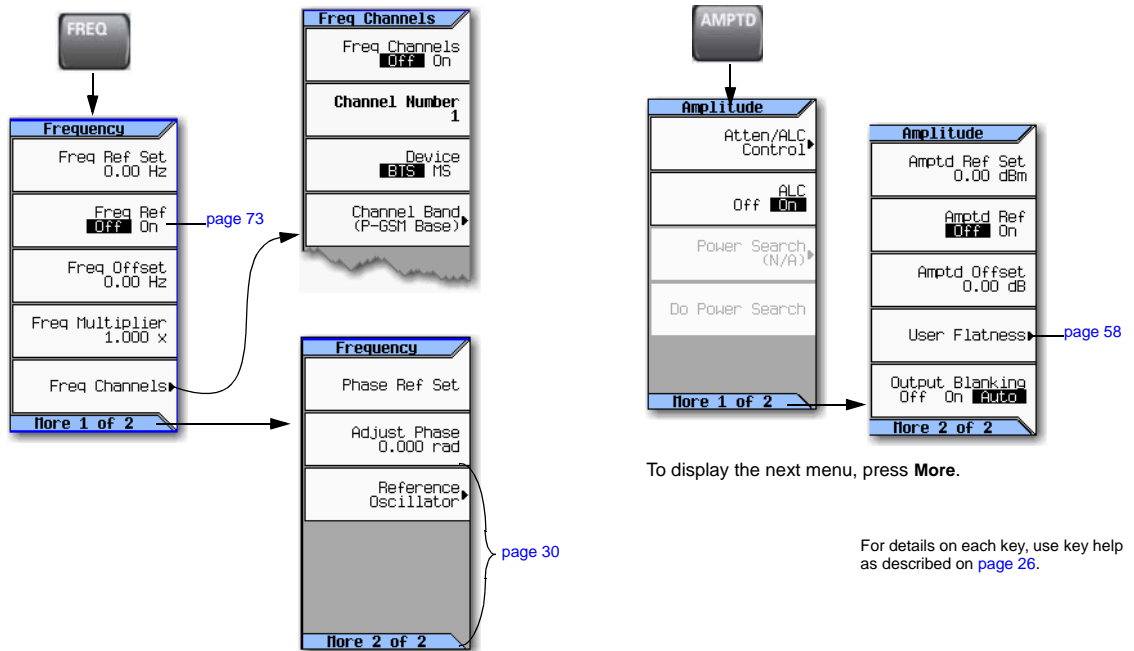

Example: Configuring a 700 MHz, -20 dBm Continuous Wave Output

1. Preset the signal generator.

The signal generator displays its maximum specified frequency and minimum power level (the front panel display areas are shown on page 8).

2. Set the frequency to 700 MHz: Press **Freq > 700 > MHz**.

The signal generator displays 700 MHz in both the FREQUENCY area of the display and the active entry area.

3. Set the amplitude to -20 dBm: Press **Amptd > -20 > dBm**.

The display changes to -20 dBm in the AMPLITUDE area of the display, and the amplitude value becomes the active entry. Amplitude remains the active function until you press another function key.

4. Turn on the RF Output: Press **RF On/Off**.

The RF Output LED lights, and a 700 MHz, -20 dBm CW signal is available at the RF OUTPUT connector.

Using an External Reference Oscillator

When using an external reference, you can select either narrow or wide bandwidth mode.

For details on each key, use key help as described on [page 26](#).

Freq > More


Int = uses the signal generator's internal reference oscillator.

Auto = uses the signal generator's internal reference unless a signal is present at the rear panel REF IN connector. If an external signal is present, that signal is used as the reference.

Range: 1 - 50 MHz
For guaranteed operation below 2 MHz, select Narrow bandwidth; in Wide bandwidth, operation using frequencies below 2 MHz is not guaranteed.

Figure 3-2 illustrates the better close in phase noise of the wide bandwidth mode. If the external reference you are using is noisy or spurious, use the narrow bandwidth mode. With Wide bandwidth selected, If you select a frequency less than 2 MHz, the signal generator displays a warning message.

Figure 3-2 Using an External Reference Oscillator

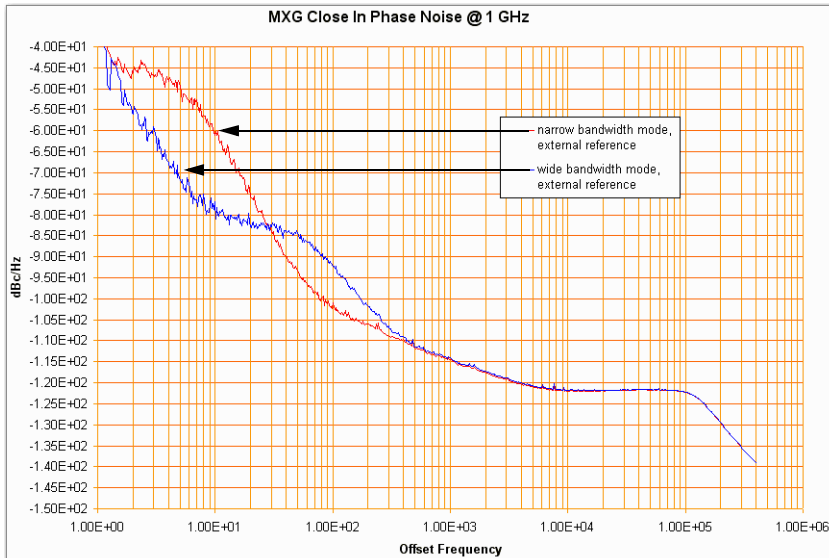


Configuring a Swept Output

The signal generator has two methods of sweeping through a set of frequency and amplitude points:

Step sweep (page 33) provides a linear or logarithmic progression from one selected frequency, amplitude, or both, to another, pausing at linearly or logarithmically spaced points (steps) along the sweep. The sweep can progress forward, backward, or manually.

List sweep (page 38) enables you to enter frequencies and amplitudes at unequal intervals, in nonlinear ascending, descending, or random order. List sweep also enables you to copy the current step sweep values, include an Arb waveform in a sweep (on a vector instrument), and save list sweep data in the file catalog (page 49).


Figure 3-3 Sweep Softkeys

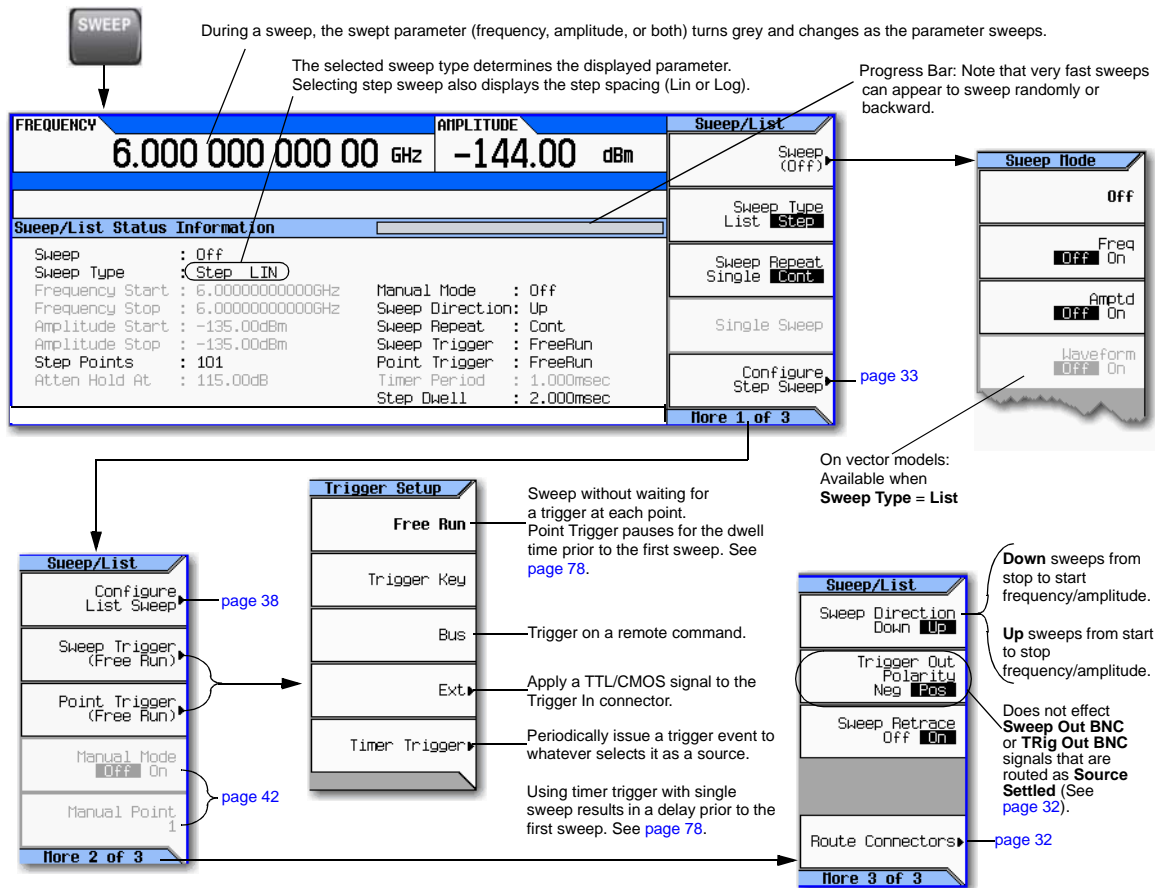

For details on each key, use key help as described on page 26.

Routing Signals

Sweep > More > More > Route Connectors

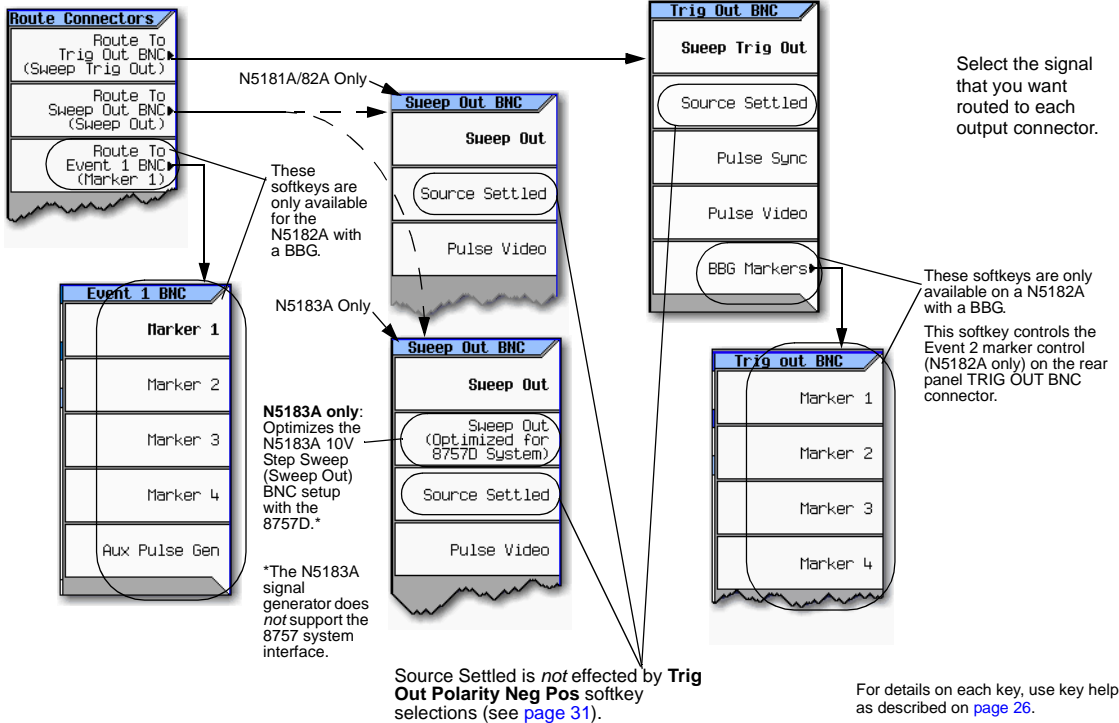


Step Sweep

Step sweep provides a linear or logarithmic progression from one selected frequency, or amplitude, or both, to another, pausing at linearly or logarithmically spaced points (steps) along the sweep. The sweep can progress forward, backward, or be changed manually.

The N5183A allows you to use step sweep along with the frequency markers on instruments during measurements (refer to “Using Frequency Markers (N5183A Only)” on page 37).

NOTE The N5183A does *not* support the 8757 system interface.

Figure 3-4 Sweep Softkeys

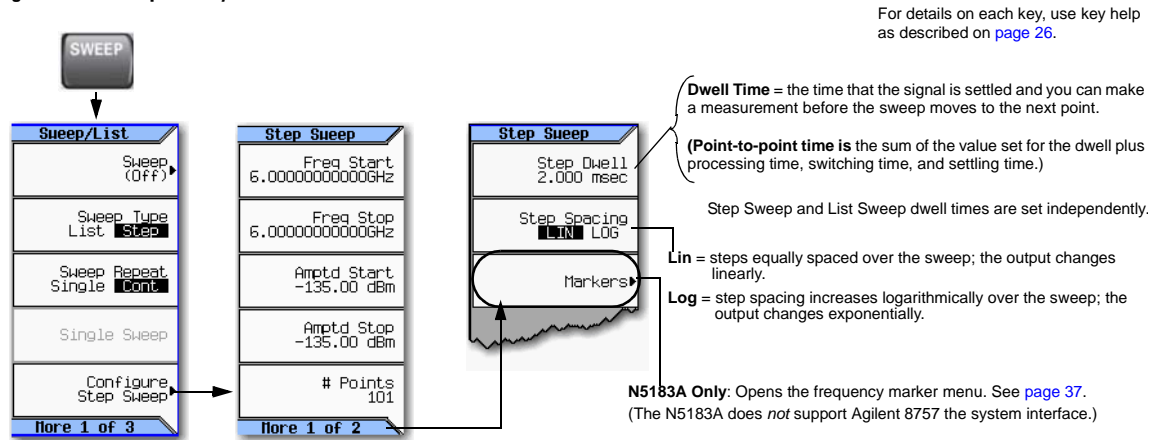

Example: Configuring a Continuous, Linear Step Sweep

Output: A signal that continuously sweeps from 500 to 600 MHz and from -20 to 0 dBm, with a dwell time of 500 ms at each of six equally-spaced points.

1. Preset the instrument and open the Sweep/List menu: Press **Preset** > **SWEEP**.
Because continuous is the default sweep repeat selection, and linear is the default step spacing selection, you do not need to set these parameters.
2. Open the step sweep menu: Press **Configure Step Sweep**.
3. Set the following parameters:

Start frequency 500 MHz:

Press **Freq Start** > **500** > **MHz**

Stop frequency 600 MHz:	Press Freq Stop > 600 > MHz
Amplitude at the beginning of the sweep, -20 dBm:	Press Amptd Start > -20 > dBm
Amplitude at the end of the sweep, 0 dBm:	Press Amptd Stop > 0 > dBm.
6 sweep points:	Press # Points > 6 > Enter
Dwell time at each point, 500 milliseconds:	Press More > Step Dwell > 500 > msec

4. Sweep both frequency and amplitude: Press **Return > Return > Sweep > Freq Off On > Amptd Off On.**

A continuous sweep begins, from the start frequency/amplitude to the stop frequency/amplitude. The *SWEEP* annunciator displays, and sweep progress is shown in the frequency display, the amplitude display, and the progress bar.

5. Turn the RF output on: Press **RF On/Off.**

The RF LED lights, and the continuous sweep is available at the RF Output connector.

Using Basic Step Sweep Functions

This procedure demonstrates the following task:

- “Configuring a Frequency Sweep” on page 35


Configuring a Frequency Sweep

For this example, we are going to set a step sweep using the N5183A, over a frequency range of 7.5 GHz to 10.0 GHz, using a band-pass filter as our device under test, and display that response on a 8757D Scalar Analyzer.

1. Set up the equipment as shown in Figure 3-5.

NOTE The N5183A signal generator does *not* support the 8757 system interface. Scalar analyzer settings *must* match the signal generator’s settings.

Figure 3-5 Equipment Setup

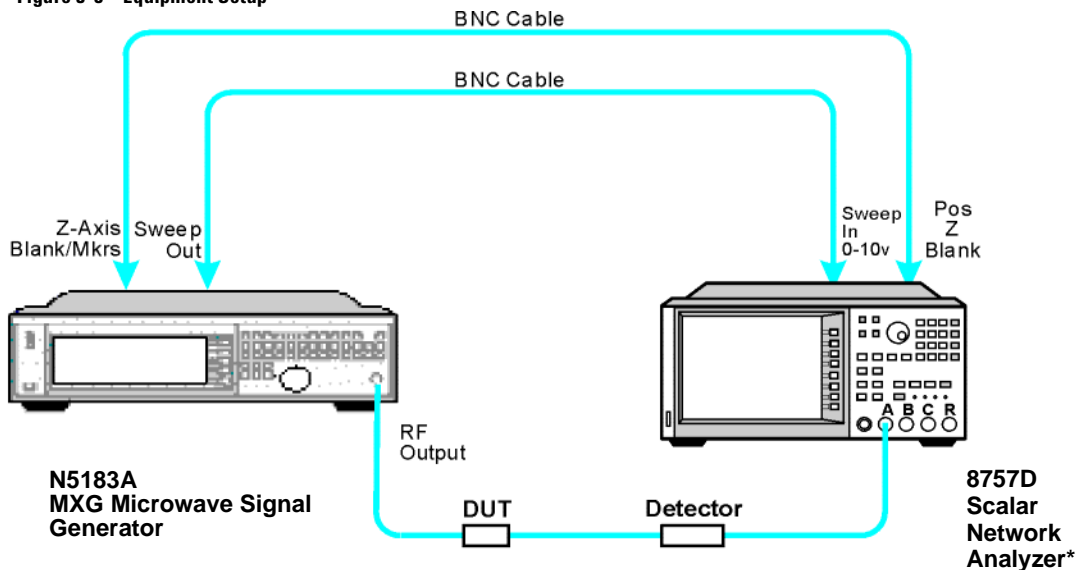

*The N5183A signal generator is not compatible with the 8757 system interface.

2. Turn on both the 8757D and the N5183A.
3. On the 8757D:
 - a. Press **SYSTEM** > **MORE** > **SWEEP MODE** and verify that the **SYSENTF** softkey is set to OFF.
 - b. Press **SYSTEM** > **MORE** > **DC**
 - c. Press **SYSTEM** > **Freq LABELS** > **START FREQ** > **7.5 GHz**
 - d. Press **SYSTEM** > **FREQ LABELS** > **STOP FREQ** > **10.0 GHz**


- e. Press **SYSTEM > TRACE # POINTS > 801**
4. On the N5183A:
 - a. Change the connector routing to 8757D System, enabling the N5183A to provide a sweep out to the 8757D during Step sweep operations. Press **Sweep > More > More > Route Connectors > Route to Sweep Out BNC > Sweep Out (Optimized for 8757D System)**.
 - b. Press **Sweep > Configure Step Sweep > # Points > 801**
 - c. Press **Sweep > Configure Step Sweep > Freq Stop > 10.0 GHz**
 - d. Press **Sweep > Configure Step Sweep > Freq Start > 7.5 GHz**
 - e. Press **Sweep > Sweep > Freq On Off** set to **On**

NOTE During swept RF output, the **FREQUENCY** and/or **AMPLITUDE** areas of the signal generator's display are *greyed out*, depending on what is being swept. In this case, since frequency is being swept the **FREQUENCY** area of the display is greyed out.

5. On the 8757D: Adjust the settings for start and stop frequency response of the device under test (DUT) so it is clearly seen on the 8757D display.

You may need to rescale the response on the 8757D for a more accurate evaluation of the amplitude. [Figure 3-6 on page 36](#) shows an example of a bandpass filter response.

Figure 3-6 Bandpass Filter Response on 8757D

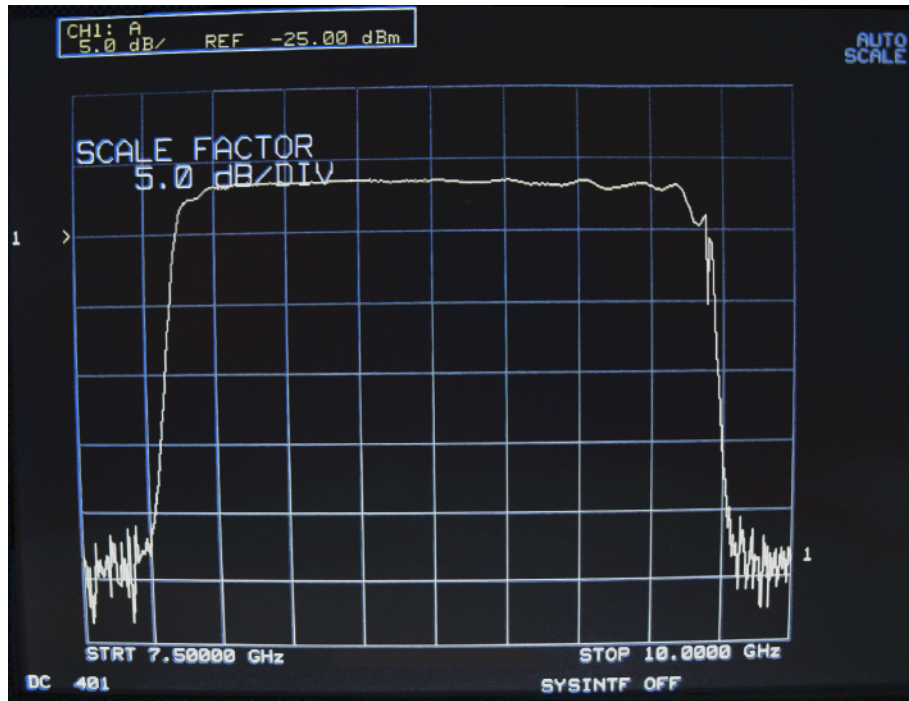

Using Frequency Markers (N5183A Only)

In step sweep mode, you can use the N5183A to create up to 20 frequency markers to display on your measurement equipment.

NOTE The N5183A does *not* support the 8757 system interface.

Figure 3-7 Frequency Marker Softkeys

Sweep > Configure Step Sweep >
More > Markers

For details on each key, use key help as described on [page 26](#).

marker	marker	Frequency	On/Off	Ref
0	40.0000000000	GHz	OFF	---
1	40.0000000000	GHz	OFF	---
2	40.0000000000	GHz	OFF	---
3	40.0000000000	GHz	OFF	---
4	40.0000000000	GHz	OFF	---
5	40.0000000000	GHz	OFF	---
6	40.0000000000	GHz	OFF	---
7	40.0000000000	GHz	OFF	---

Marker Freq ← Sets the frequency for the marker number highlighted. Up to 20 frequency markers can be set.

Marker On/Off ← Enables the selected frequency marker.

Delta Ref Set ← Selects the highlighted marker as the frequency reference marker for the rest of the frequency markers.

Turn Off Markers ← If the **Delta Ref Set** softkey has been pressed, this softkey enables the **Marker Delta** function and uses the Ref marker as the frequency marker reference for the other markers.

Marker->Center Freq ← Sets the center frequency of the sweep to the value of the highlighted marker (row).


M1->Start M2->Stop ← Sets the start frequency of the sweep to the value of marker 1 (M1) and the stop frequency to the value of marker 2 (M2).

Marker Amplitude ← Sets the marker's amplitude value displayed on the instrument (Range: -10 dB to 10 dB).

List Sweep

List sweep enables you to enter frequencies and amplitudes at unequal intervals in nonlinear ascending, descending, or random order. List sweep also enables you to copy the current step sweep values, include a waveform in a sweep (on a vector instrument), and save list sweep data in the file catalog (page 49). Dwell time is editable at each point. For fastest switching speeds, use list sweep.

Figure 3-8 List Sweep Configuration Softkeys and Display

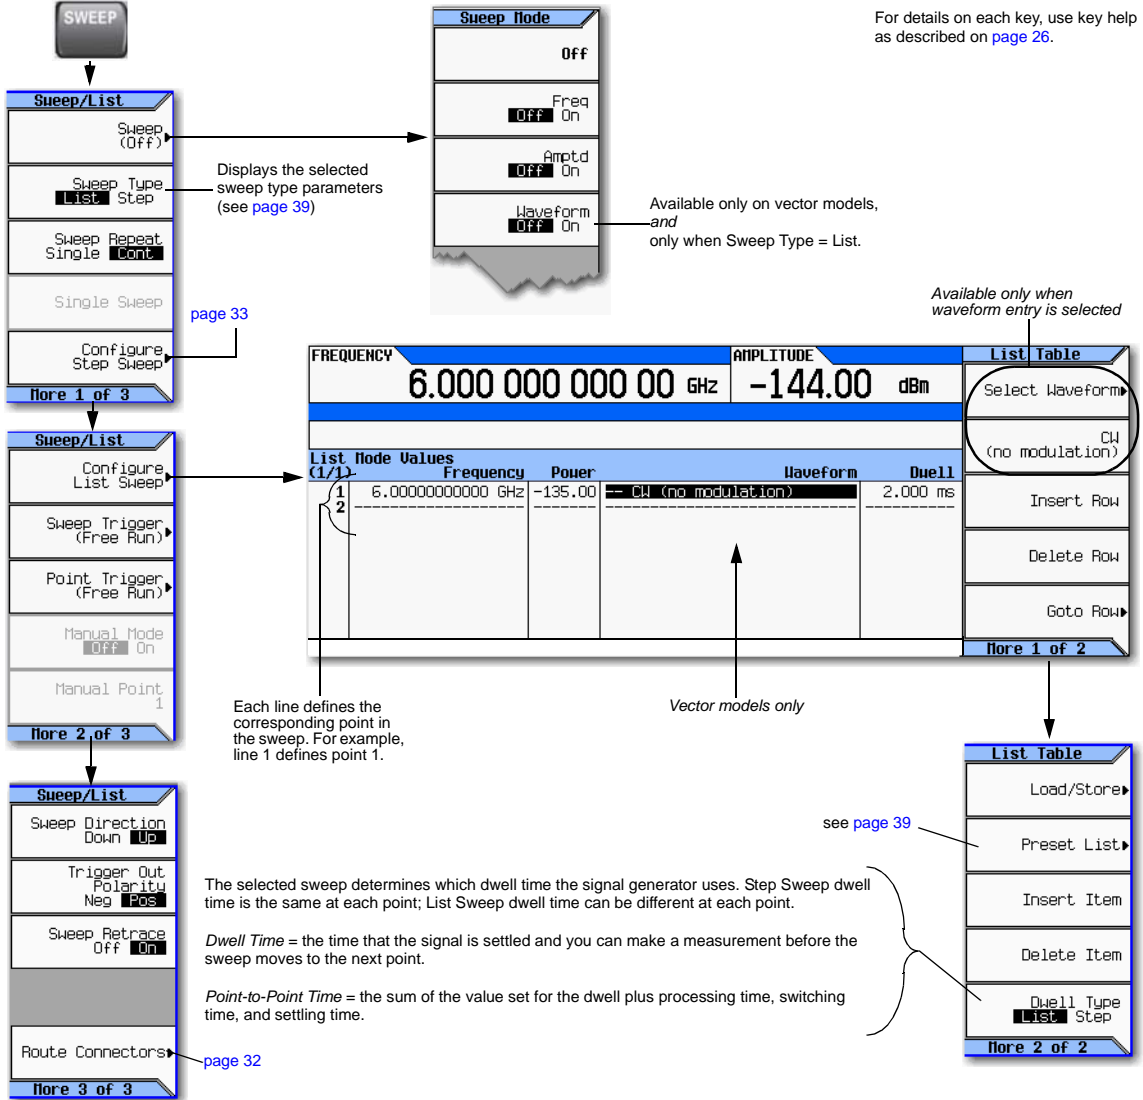

Example: Configuring a List Sweep Using Step Sweep Data

1. Set up the desired step sweep, but do not turn the sweep on. This example uses the step sweep configured on [page 33](#).
2. In the SWEEP menu, change the sweep type to list:
Press **SWEEP > Sweep Type List Step** to highlight List.

The display shows sweep list parameters, as shown below.

FREQUENCY	AMPLITUDE	Sweep/List
6.000 000 000 00 GHz	-144.00 dBm	Sweep (Off) ▶
Sweep/List Status Information		Sweep Type List Step
Sweep : Off	Current Point : 0/1	Sweep Repeat Single Cont
Sweep Type : List	Sweep Speed : Opts/sec	Single Sweep
Frequency Points: 1	Manual Mode : Off	Configure Step Sweep ▶
Amplitude Points: 1	Sweep Direction: Up	More 1 of 3
Waveform Points : 1	Sweep Repeat : Cont	
Dwell Points : 1	Sweep Trigger : FreeRun	
Dwell Type : List	Point Trigger : FreeRun	
Atten Hold At : 115.00dB	Timer Period : 1.000msec	
	Step Dwell : 500.000msec	

3. Open the List Sweep menu: Press **More > Configure List Sweep**.
4. Clear any previously set values from the menu and load the points defined in the step sweep into the list: Press **More > Preset List > Preset with Step Sweep > Confirm Preset**.

The display updates with the values loaded from the step sweep, as shown.

FREQUENCY	AMPLITUDE	List Table			
6.000 000 000 00 GHz	-144.00 dBm	Load/Store ▶			
List Node Values (1/1)		Preset List ▶			
1	500.000000000000 MHz	-20.00	-- CW (no modulation)	500.000 ms	Insert Item
2	520.000000000000 MHz	-16.00	-- CW (no modulation)	500.000 ms	Delete Item
3	540.000000000000 MHz	-12.00	-- CW (no modulation)	500.000 ms	Dwell Type List Step
4	560.000000000000 MHz	-8.00	-- CW (no modulation)	500.000 ms	More 2 of 2
5	580.000000000000 MHz	-4.00	-- CW (no modulation)	500.000 ms	
6	600.000000000000 MHz	+0.00	-- CW (no modulation)	500.000 ms	
7			Waveforms are available only on vector models.		

Vector Models:

Presetting the list clears any previously selected waveforms.

For information on selecting a list sweep waveform, see [Example: Editing List Sweep Points](#) on page 40.

5. Sweep frequency and amplitude: Press **SWEEP (hardkey) > Sweep > Freq Off On > Amptd Off On**.
Setting the sweep turns on the sweep function; a continuous sweep begins. On the display, the SWEEP annunciator appears, and the progress bar shows the progression of the sweep.
6. If not already on, turn the RF output on: Press **RF On/Off**.
The RF Output LED lights, and a continuous sweep is available at the RF OUTPUT connector.

Example: Editing List Sweep Points

If you are not familiar with table editors, refer to [page 28](#).

1. Create the desired list sweep. This example uses the list sweep created in the previous example.
2. If sweep is on, turn it off. Editing list sweep parameters with sweep on can generate an error.
3. Ensure that the sweep type is set to list: Press **SWEEP > Sweep Type List Step** to highlight List.
4. In the List Mode Values table editor, change the point 1 dwell time (defined in row 1) to 100 ms:
 - a. Press **More > Configure List Sweep**.
 - b. Highlight the point 1 dwell time.
 - c. Press **100 > msec**.

The next item in the table (the frequency value for point 2) highlights.

5. Change the selected frequency value to 445 MHz: Press **445 > MHz**.
6. Add a new point between points 4 and 5: Highlight any entry in row 4 and press **Insert Row**.
This places a copy of row 4 below row 4, creating a new point 5, and renumbers subsequent rows.
7. Shift frequency values down one row, beginning at point 5: Highlight the frequency entry in row 5, then press **More > Insert Item**.

This places a copy of the highlighted frequency value in row 6, shifting the original frequency values for rows 6 and 7 down one row. The new row 8 contains only a frequency value (the power and dwell time entries do not shift down).

8. Change the still-active frequency value in row 5 to 590 MHz: Press **590 > MHz**. The power in row 5 is now the active parameter.
9. Insert a new power value (-2.5 dBm) for point 5, and shift down the original power values for points 5 and 6 by one row: Press **Insert Item > -2.5 > dBm**.
10. To complete the entry for point 8, insert a duplicate of the point 7 dwell time by shifting a copy of the existing value down: Highlight the dwell time in row 7 and press **Insert Item**.
11. *For an analog instrument, go to step 14.* For a vector instrument, continue with step 12.
12. Select a waveform for point 2:
 - a. Highlight the waveform entry for point 2 and press the **More > Select Waveform**.
The signal generator displays the available waveforms, as shown in the following example.

Select (1/1)	Segment On BBG Media	Points	Sequence On Int Media	Segs
	RAMP_TEST_WF1	200	A	4
	SINE_TEST_WF1	200		

- b. Highlight the desired waveform (in this example, SINE_TEST) and press either the **Select** hardkey or the **Select Waveform** softkey.

13. As desired, repeat step 12 for the remaining points for which you want to select a waveform. The following figure shows an example of how this might look.

FREQUENCY		AMPLITUDE		List Table	
6.000 000 000 00 GHz		-144.00 dBm		Edit Item	
List Node Values (1/1)					
Frequency	Power	Waveform	Dwell	Insert Row	
1 500.00000000000 MHz	-20.00	-- CW (no modulation)	100.000 ms	Delete Row	
2 445.00000000000 MHz	-16.00	WFM1:SINE_TEST_WFM	500.000 ms	Goto Row	
3 540.00000000000 MHz	-12.00	-- CW (no modulation)	500.000 ms		
4 560.00000000000 MHz	-8.00	-- CW (no modulation)	500.000 ms		
5 590.00000000000 MHz	-2.50	WFM1:RAMP_TEST_WFM	500.000 ms		
6 560.00000000000 MHz	-8.00	WFM1:RAMP_TEST_WFM	500.000 ms		
7 580.00000000000 MHz	-4.00	-- CW (no modulation)	500.000 ms		
8 600.00000000000 MHz	+0.00		500.000 ms		
9					
Page 1 of 2					

The empty entry is equivalent to choosing CW (no modulation).

14. Turn sweep on:

Press **Return** > **Return** > **Return** > **Sweep** > **Freq Off On** > **Amptd Off On** > **Waveform Off On**.

15. If it is not already on, turn the RF output on:

Press **RF On/Off**.

The SWEEP annunciator appears on the display, indicating that the signal generator is sweeping, and the progress bar shows the progression of the sweep.

NOTE If the instrument is in manual sweep (page 42), the active row (row 6 in the figure above) is the selected (manual) point, and the signal generator outputs the settings for that selection when the RF output is on.

Example: Using a Single Sweep

1. Set up either a step sweep (page 33) or a list sweep (page 39).

2. In the List/Sweep menu, set the sweep repeat to single:

Press **Sweep Repeat Single Cont** to highlight Single.

Sweep does not occur until you trigger it.

Note that the WINIT annunciator appears on the display, indicating that the sweep is waiting to be initiated.

3. If not already on, turn the RF output on: Press **RF On/Off**.

4. Initiate the sweep: Press **Single Sweep**.

A single repetition of the configured sweep is available at the RF Output connector.

As the signal generator sweeps, the SWEEP annunciator replaces WINIT on the display, and the progress bar shows the progression of the sweep.

At the end of the sweep, there is no progress bar, and the WINIT annunciator replaces SWEEP.

Example: Manual Control of Sweep

1. Set up either a step sweep (page 33) or a list sweep (page 39).
2. In the Sweep/List menu, select a parameter to sweep: Press **Sweep** > *parameter* > **Return**.
3. Select manual mode: Press **More** > **Manual Mode Off On**.

When you select manual mode, the current sweep point becomes the selected manual point.

4. If it is not already on, turn the RF output on: Press **RF On/Off**.
5. Select the desired point to output: Press **Manual Point** > *number* > **Enter**.

The progress bar changes to indicate the selected point.

6. Use the knob or arrow keys to move from point to point. As you select each point, the RF output changes to the settings in that selection.

The screenshot shows the instrument's interface with the following elements and annotations:

- SWMAN annunciator:** Located at the top left, indicating manual mode.
- Current Sweep Point:** A progress bar and 'Current Point : 3/6' indicator showing the selected point.
- Manual Point:** A field showing 'Manual Point: 3'.
- Parameters:** Frequency (540.000 000 00 MHz) and Amplitude (-144.00 dBm).
- Manual Mode:** A toggle switch currently set to 'On'.

Annotations provide further context:

- "The SWMAN annunciator indicates that the sweep is in manual mode."
- "The currently sweeping parameter stops and displays the selected point."
- "When you enter a manual point, the progress bar moves to and stops at the selected point."
- "The parameters of the selected sweep point (point 3 of 6 in this example) define the signal available at the RF Output connector."
- "When you turn manual mode on, the current sweep point becomes the manual point."

Sweep/List Status Information	
Sweep	: Freq
Sweep Type	: Step LIN
Frequency Start	: 500.00000000MHz
Frequency Stop	: 600.00000000MHz
Amplitude Start	: -20.00dBm
Amplitude Stop	: 0.00dBm
Step Points	: 6
Atten Hold At	: 115.00dB
Current Point	: 3/6
Sweep Speed	: 0pts/sec
Manual Mode	: On
Sweep Direction	: Up
Sweep Repeat	: Cont
Sweep Trigger	: FreeRun
Point Trigger	: FreeRun
Timer Period	: 1.000msec
Step Dwell	: 500.000msec

Modulating the Carrier Signal

To modulate the carrier signal, you must have both

- an active modulation format
and
- modulation of the RF output enabled

Example

1. Preset the signal generator.
2. Turn on AM modulation: Press **AM > AM Off On** (requires Option UNT).

You can turn on the modulation format before or after setting signal parameters.

The modulation format generates, but does not yet modulate the carrier signal.

Once the signal generates, an annunciator showing the name of the format appears, indicating that a modulation format is active.

3. Enable modulation of the RF output: Press the **Mod On/Off** key until the LED lights.

If you enable modulation without an active modulation format, the carrier signal does not modulate until you subsequently turn on a modulation format.

Annunciator indicates active AM modulation

Mod	State	Depth/Dev	Source	Rate	Waveform
AM	Mod Off	0.1%	Internal	400.0Hz	Sine
FH	Off	1.000kHz	Internal	400.0Hz	Sine
PM	Off	0.000rad	Internal	400.0Hz	Sine
Pulse	Off	1.00us	Internal	2.00us	Free-Run
Burst	Off		Int		
I/Q	Off		Internal		

NOTE To turn modulation *off*, press the **Mod On/Off** key until the LED turns off.

When the **Mod On/Off** key is off, the carrier signal is not modulated, even with an active modulation format.

4. To make the modulated carrier available at the RF output connector, press the **RF On/Off** key until the LED lights.

See also: “Using Analog Modulation (Option UNT Only)” on page 81
“Using Pulse Modulation (Option UNU or UNW)” on page 85
“I/Q Modulation” on page 152

Simultaneous Modulation

NOTE The Agilent MXG is capable of simultaneous modulation. All modulation types (AM, FM, ϕ M, and Pulse) may be simultaneously enabled. But, there are some exceptions. Refer to [Table 3-1](#).

Table 3-1 Simultaneous Modulation Type Combinations

	AM ^a	FM	ϕ M	Pulse ^b
AM	--	x	x	x
FM	x	--	<i>not applicable</i>	x
ϕ M	x	<i>not applicable</i>	--	x
Pulse	x	x	x	--

^aLinear AM and Exponential AM *cannot* be enabled simultaneously. Refer to [Chapter 5](#).

^bPulse modulation requires Option UNU or UNW. Refer to [Chapter 6](#).

Working with Files


- [File Softkeys](#) on page 46
- [Viewing a List of Stored Files](#) on page 47
- [Storing a File](#) on page 48
- [Loading \(Recalling\) a Stored File](#) on page 49
- [Moving a File from One Media to Another](#) on page 50
- [Working with Instrument State Files](#) on page 51
- [Selecting the Default Storage Media](#) on page 55

The signal generator recognizes several types of files, such as instrument state files, license files, and list sweep files. Files can be stored either in the signal generator's internal storage or on the USB media. This section provides an overview of how to navigate the signal generator's file menus, and how to view, store, load, and move files.

See also: [Storing, Loading, and Playing a Waveform Segment](#) on page 98.

File Softkeys

For details on each key, use key help as described on [page 26](#).

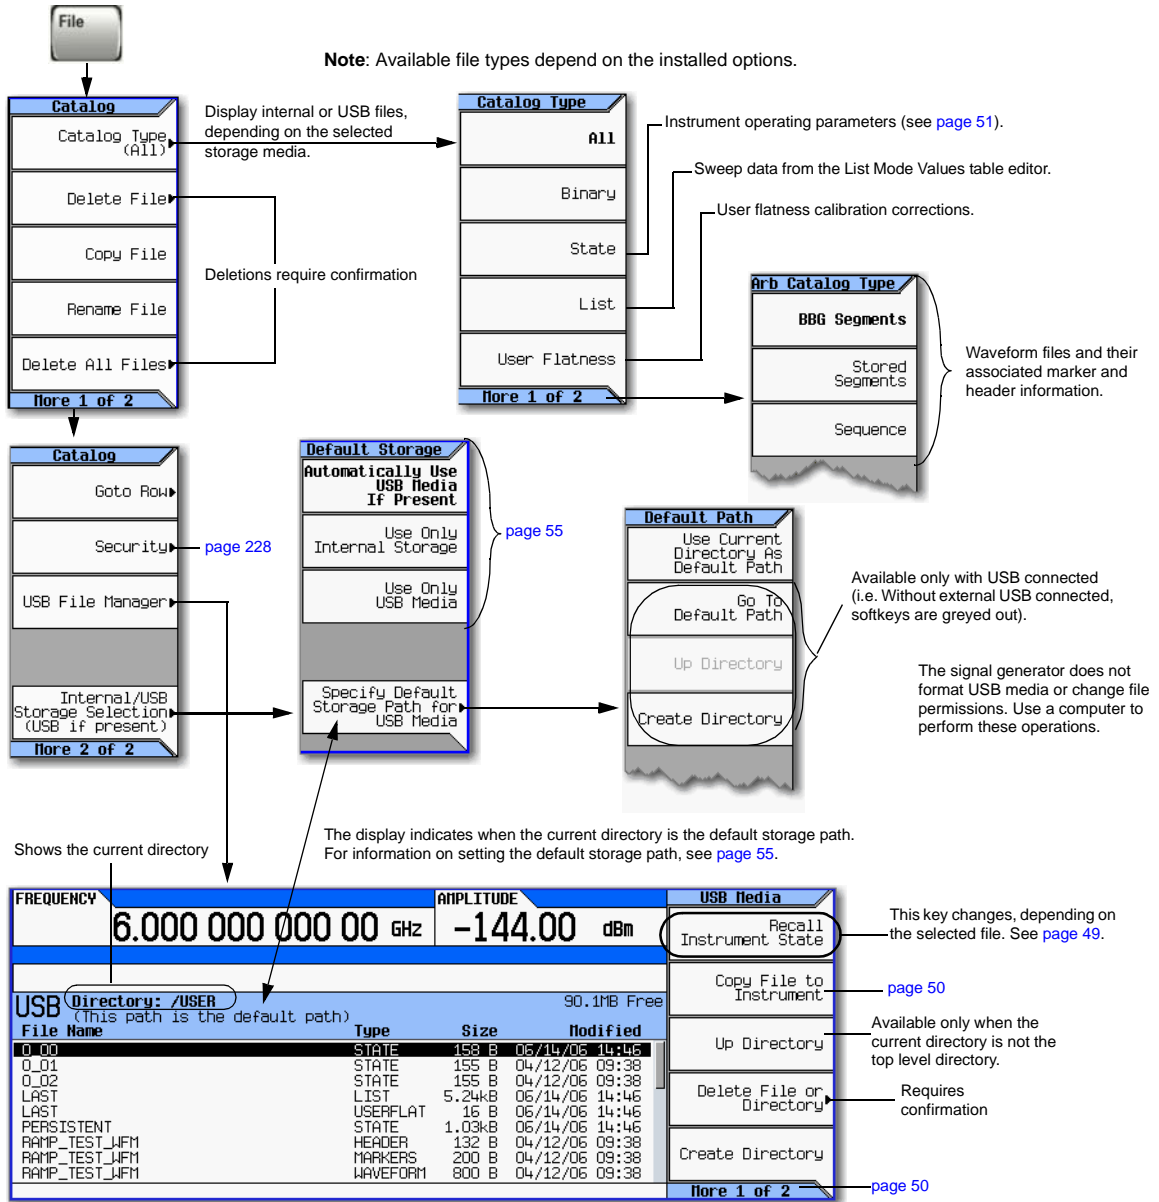

When you connect USB media to the instrument, the signal generator displays the USB Media menu and the message **External USB Storage attached**. When you disconnect the USB media, the message **External USB Storage detached** displays. When you open the External Media menu without USB media connected, the signal generator displays the message **External Media Not Detected**.

Viewing a List of Stored Files

The information in this section is provided with the assumption that default storage media is set to Auto, as described on [page 55](#).

Viewing a List of Files Stored in the Signal Generator

1. If USB media is connected, disconnect it. The signal generator's storage media switches to internal, so you can now use the file catalogs to see files stored in the signal generator.
2. Select the desired file catalog: Press **File > Catalog Type > desired catalog** (in this example, **All**). The selected files appear in alphabetical order by file name, as shown in the following figure.

The selected file catalog and the storage media

File Name	Type	Size	Modified
1 120456789_23045789_12345	LIST	5359	06/07/06 10:34
2 12TONE_WFM	SNVWFM	10752	09/22/06 22:36
3 1A	SEQ	539	10/31/06 09:15
4 2_00	STATE	201	11/02/06 10:05
5 BOGUS	LIST	69	09/22/06 22:36
6 BOGUS	NVWKR	69	10/09/06 14:41
7 BOGUS.IT	LIST	69	09/22/06 22:36
8 CDMA2K_SCHAN_WFM	SNVWFM	1474752	09/22/06 22:36
9 CDMA2K_PILOT_WFM	SNVWFM	1474752	09/22/06 22:36
10 DISPLAY.BMP	BINARY	76918	09/22/06 22:36

Viewing a list of Files Stored on USB Media

With USB media connected, you can view files on USB media using either the file catalogs, which can display only a selected type of file, or the USB File Manager, which displays all files.

Using the File Catalogs:

- With the USB media connected, select the desired file catalog: press **File > Catalog Type > desired catalog**. The selected files appear in alphabetical order by file name.

Using the USB File Manager:

- With USB media connected, open the USB File Manager: press **File > More > USB File Manager**. The instrument displays the default directory on the USB Media, as shown in the following figure. Note that when you attach USB media, the display goes directly to this menu.

Use the **Page Up** and **Page Down** hardkeys to scroll through the contents of the directory.


File Name	Type	Size	Modified
0_00	STATE	158 B	06/14/06 14:46
0_01	STATE	155 B	04/12/06 09:38
0_02	STATE	155 B	04/12/06 09:38
LAST	LIST	5.24kB	06/14/06 14:46
LAST	USERFLAT	16 B	06/14/06 14:46
PERSISTENT	STATE	1.03kB	06/14/06 14:46
RAMP_TEST_WFM	HEADER	132 B	04/12/06 09:38
RAMP_TEST_WFM	MARKERS	200 B	04/12/06 09:38
RAMP_TEST_WFM	WAVEFORM	800 B	04/12/06 09:38

Storing a File

Several menus enable you to store instrument parameters. For example, you can store instrument states, lists, and waveforms.

- An instrument state file contains instrument settings. For this type of file, use the **Save** hardkey shown in [Figure 3-9 on page 51](#).
- For other types of data, use the **Load/Store** softkey (shown below) that is available through the menu used to create the file.

File Type	Save From
List	Sweep menu
State	Save menu
Waveform	Mode menu
User Flatness	Amplitude menu
User Preset	User Preset menu

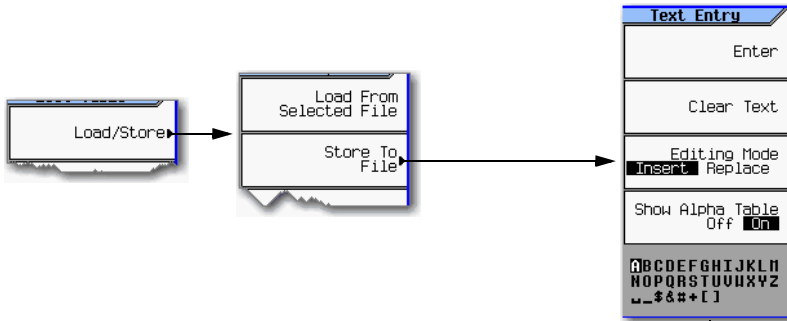

Use this menu to enter the file name, as described on [page 27](#).


File Length (including extension)
Internal Media: 25 characters
USB Media: 39 characters

For details on each key, use key help as described on [page 26](#).

Loading (Recalling) a Stored File

There are several ways to load (recall) a stored file.

- For an instrument state file, use the **Recall** hardkey shown in [Figure 3-9 on page 51](#).
- For other types of data, use the Load/Store softkey (shown below) that is available through the menu used to create the file.

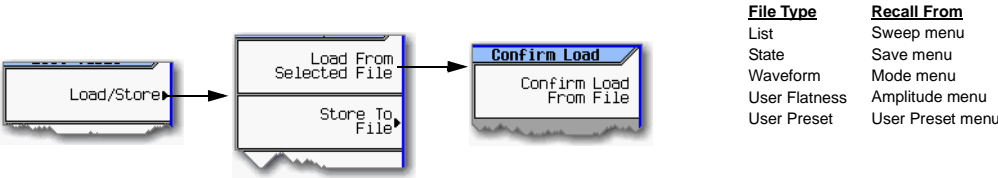


Loading a File From USB Media

To load a file from USB media, use the USB file manager shown below.

File > Catalog Type > <type> > More > USB File Manager
 or
File > More > USB File Manager
 or
 Insert the USB media

<u>File Type</u>	<u>Extension</u>	<u>Pressing Select with file highlighted...</u>
List	.list	loads list and starts sweep
State	.state	load instrument state
Waveform	.waveform	loads and plays waveform
User Flatness	.uflat	loads and applies user flatness
User Preset	.uprst	loads and executes user preset
License	.lic	installs purchased license

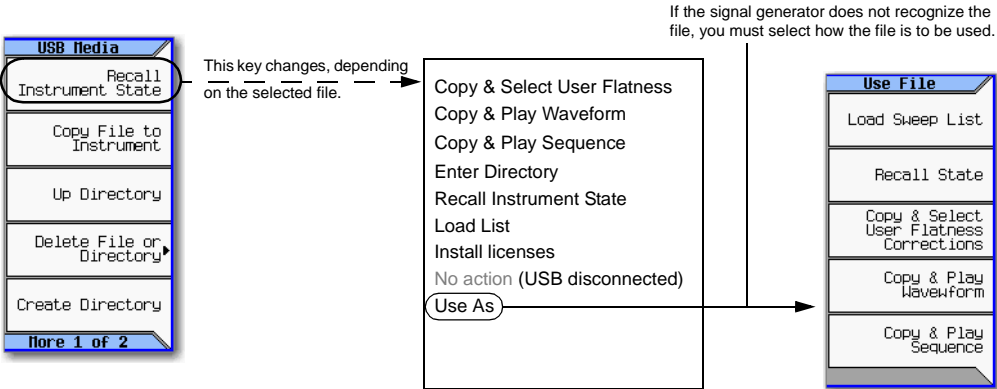

For details on each key, use key help as described on [page 26](#).

Moving a File from One Media to Another

Use the USB Media Manager to move files between USB and internal media.


File > Catalog Type > <type> > More > USB File Manager

or

File > More > USB File Manager

or

Insert the USB media

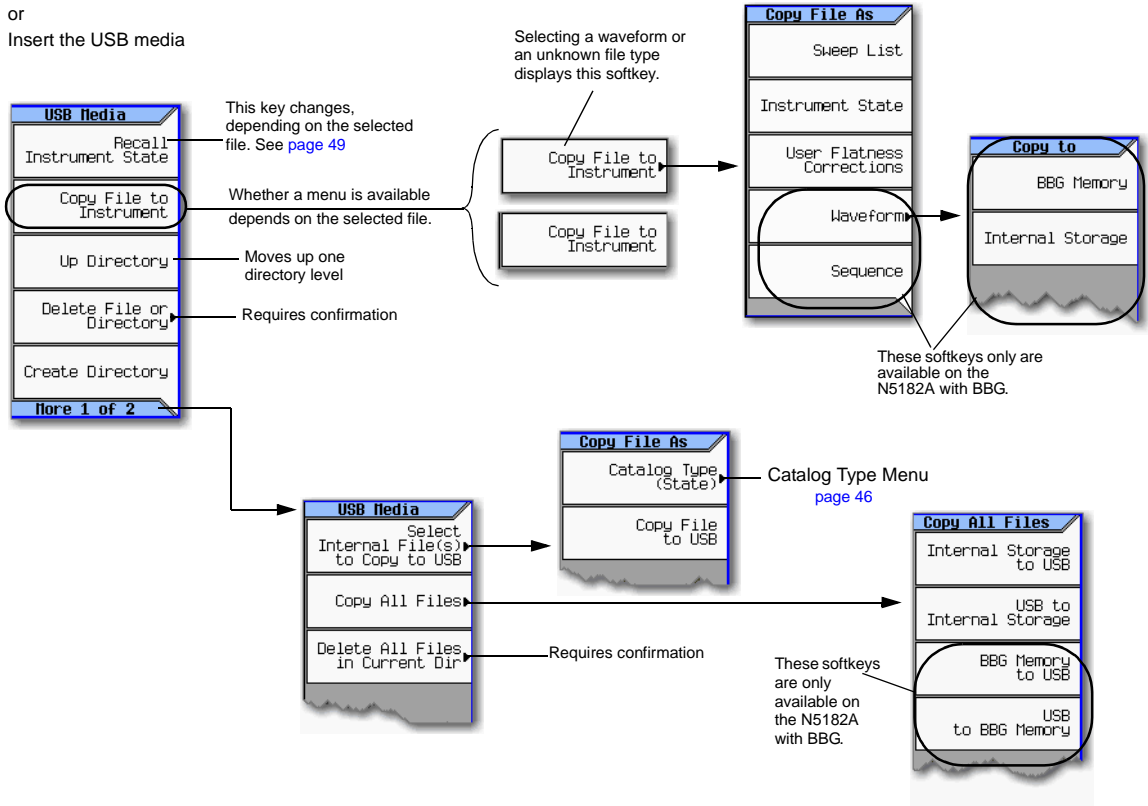


For details on each key, use key help as described on [page 26](#).

Working with Instrument State Files

- [Saving an Instrument State](#) on page 52.
- [Saving a User Preset](#) on page 52.
- [Recalling an Instrument State](#) on page 52.
- [Recalling an Instrument State and Associated Waveform File](#) on page 53.
- [Recalling an Instrument State and Associated List File](#) on page 53.
- [Moving or Copying a Stored Instrument State](#) on page 54.

Figure 3-9 Save and Recall Softkeys

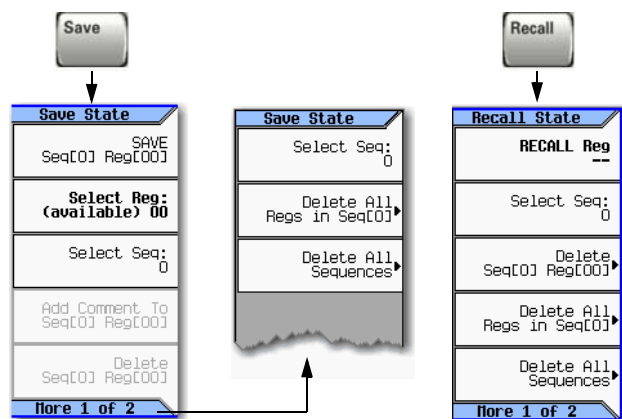

For details on each key, use key help as described on [page 26](#).

When saved to the signal generator, instrument settings (states) save to instrument state memory. Instrument state memory is divided into 10 sequences (0 through 9); each sequence comprises 100 registers (00 through 99).

Delete softkeys in the **Save** and **Recall** menus enable you to delete the contents of a specific register, or the contents of all sequences in the state file catalog.

The signal generator requires that you confirm a deletion.

The following information is *not* stored in a state file:

System Security Level	List Mode Freq	Hostname	Remote Language	FM Deviation
System Security Level Display	List Mode Power	IP Address	FTP Server	PM Deviation
System Security Level State	List Mode Dwell	Subnet Mask	Manual DHCP	MAC
Web Server (HTTP)	List Mode Sequence	Default Gateway	VXI-11 SCPI	User Power Correction
Sockets SCPI (TELNET)	Display State On/Off	ARB Files	List Files	I/Q Calibration Data

Saving an Instrument State

1. Preset the signal generator and set the following:
 - Frequency: 800 MHz
 - Amplitude: 0 dBm
 - RF: on
2. (Optional, vector models only) Associate a waveform file with these settings:
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. Highlight the desired file and press **Select Waveform**. If the file is not listed, you must first move it from internal or external media to BBG media, see [page 98](#).
3. Select the desired memory sequence (for this example, 1): Press **Save > Select Seq > 1 > Enter**.
4. Select the desired register (in this example, 01): Press **Select Reg > 1 > Save Reg**.

If a waveform is currently selected, saving the instrument state also saves a pointer to the waveform file *name*.

5. Add a descriptive comment to sequence 1 register 01:

Press **Add Comment to Seq[1] Reg[01]**, enter the comment and press **Enter**. The comment appears in the Saved States list when you press **Recall**. If the instrument state has an associated waveform, entering the waveform name in the comment makes it easy to identify which instrument state applies to which waveform.

Saving a User Preset

A user preset is a special type of instrument state file.

1. Preset the signal generator and set as desired.
2. Press **User Preset > Save User Preset**.

This saves a state file named USER_PRESET, which the signal generator recognizes as containing user preset information.

You can set up several preset conditions under different names:

1. After you save a user preset, rename it to something other than USER_PRESET (see [page 54](#)).
2. Save as many user presets as you wish, renaming the USER_PRESET file each time.
3. Give the desired file the name USER_PRESET.

Recalling an Instrument State

1. Preset the signal generator.
2. Press **Recall**.

The **Select Seq** softkey shows the last sequence used, and the display lists any states stored in the registers in that sequence; **RECALL Reg** is the active entry.

3. Select the desired instrument state:

If the desired state is listed in the currently selected sequence, press *desired number* > **Enter**.
If not, press **Select Seq > desired number > Enter > RECALL Reg > desired number > Enter**.

Recalling an Instrument State and Associated Waveform File

1. Ensure that the desired waveform file exists, and that it is in BBG media ([page 98](#)).

If the waveform file is not in BBG media, this procedure generates an error.

Recalling an instrument state with an associated waveform file recalls only the waveform *name*. It does not recreate the waveform file if it was deleted, or load the file into BBG media if it is in internal or USB media.

2. Recall the desired instrument state (see previous example).
3. View the waveform file name recalled with the instrument state: press **Mode > Dual ARB**.

The name is displayed as the selected waveform.

4. Turn on the waveform file: Press **Mode > Dual ARB > ARB Off On**.

Recalling an Instrument State and Associated List File

Recalling an instrument state recalls only the list sweep setup. It does not recall the frequency and/or amplitude values. Because you must load the list file from the file catalog, when you store a list file, be sure to give it a descriptive name (up to 25 characters).

1. Recall the desired instrument state (see previous example).
2. Load the desired list file:
 - a. Press **Sweep > More > Configure List Sweep > More > Load/Store**.
 - b. Highlight the desired file and press **Load From Selected File > Confirm Load From File**.

Editing The Comment on an Instrument Comment


Use the following steps to change a comment on an instrument state saved using the **Save** key. This is *not* the file name that appears in the State catalog (which is the file's memory location).

1. Press **Save**
2. Highlight the desired register
3. Press **Edit Comment In Seq[n] Reg [nn]**.
4. Press **Re-SAVE Seq[n] Reg[nn]**.

This overwrites previously saved instrument state settings with the new comment.

Moving or Copying a Stored Instrument State

Figure 3-10 Instrument State File Catalog

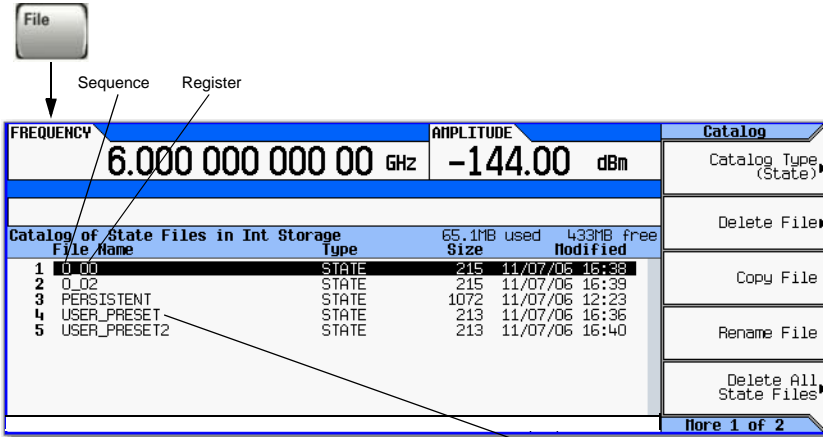

The signal generator recognizes only the file named USER_PRESET as user preset information (page 52).

A user-created state file's default name is its memory location (sequence and register).


To move the file, rename it to the desired sequence and register; you can not give a file the same name as an existing file. If you rename a state file to something other than a valid sequence/register name, the file does not appear in either the Save or Recall menu.

Selecting the Default Storage Media

You can configure the signal generator to store user files to either the internal storage or to external USB media. To automatically switch between USB media and internal storage, depending on whether USB media is attached, select **Automatically Use USB Media If Present**. To avoid storing any confidential information in the instrument, select **Use Only USB Media**. To avoid storing any confidential information to USB media, select **Use Only Internal Storage**.

This selection is unaffected by power-cycle or preset.

File > More >

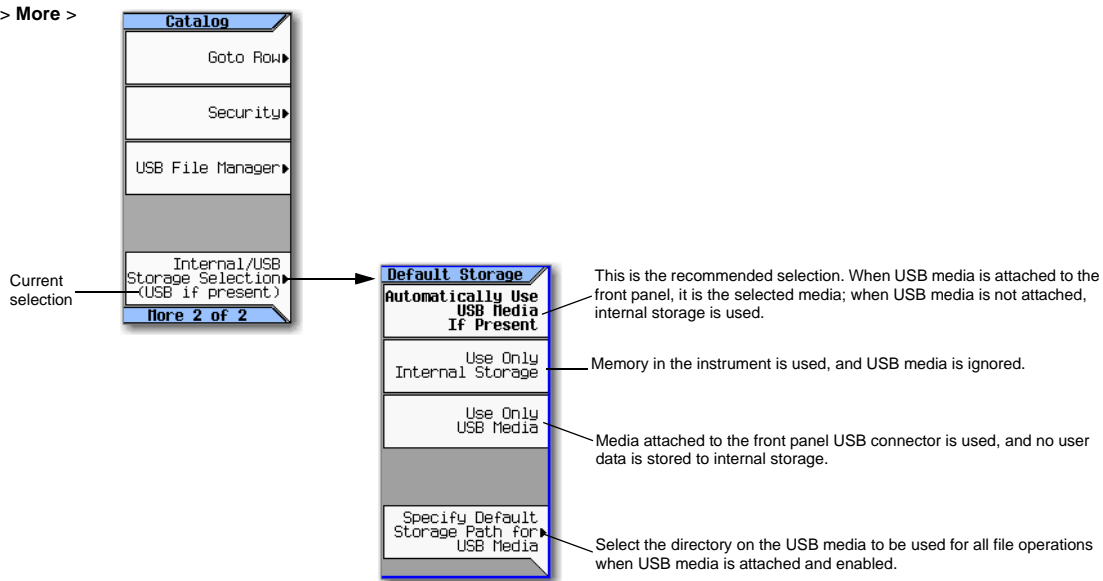

For details on each key, use key help as described on [page 26](#).

Reading Error Messages


If an error condition occurs, the signal generator reports it to both the front panel display error queue and the SCPI (remote interface) error queue. These two queues are viewed and managed separately; for information on the SCPI error queue, refer to the *Programming Guide*.

Characteristic	Front Panel Display Error Queue
Capacity (#errors)	30
Overflow Handling	Drops the oldest error as each new error comes in.
Viewing Entries	Press: Error > View Next (or Previous) Error Page
Clearing the Queue	Press: Error > Clear Error Queue(s)
Unresolved Errors ^a	Re-reported after queue is cleared.
No Errors	When the queue is empty (every error in the queue has been read, or the queue is cleared), the following message appears in the queue: No Error Message(s) in Queue 0 of 0

^aErrors that must be resolved. For example, unlock.

Error Message Format

In the front panel display error queue, error messages display on an enumerated (“1 of N”) basis.

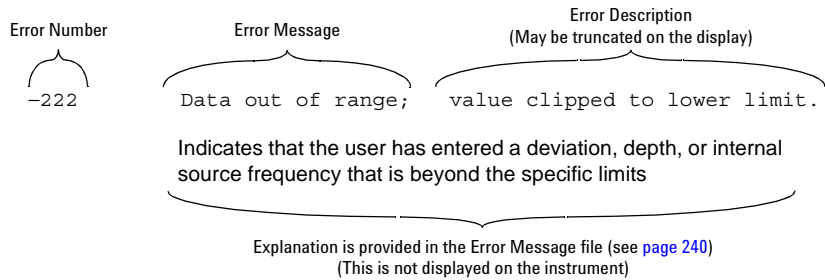

The annunciator indicates an unviewed message.

new indicates a message generated since messages were last viewed.

Modulation Status Information

Mod	State	Depth/Dev	Source	Rate	Wavefo
AM	Off	0.1%	Internal	400.0Hz	Sine
FM	On	1.000kHz	Internal	400.0Hz	Sine
PM	Off	0.000rad	Internal	400.0Hz	Sine
Pulse	Off	2.00us	Internal	4.00us	Freq
Burst	Off		Int		
I/Q	Off		Internal		

ERROR: -221, Settings conflict

Error Queue

-221, Settings conflict: Enabled modulation source conflicts with previously enabled modulation source. Previous modulation 1 of 1 disabled.

View Previous Error Page

View Next Error Page

Clear Error Queue(s)

*** PROTO CODE *** NOT FOR CUSTOMER USE *** 04/05/2006 10:12

Error messages appear in the lower-left corner of the display as they occur.

4 Optimizing Performance

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting the power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

- [Using Flatness Correction](#) on page 58
- [Using External Leveling](#) on page 67
- [Using Unleveled Operating Modes](#) on page 73
- [Using an Output Offset, Reference, or Multiplier](#) on page 75
- [Using Free Run, Step Dwell, and Timer Trigger](#) on page 78
- [Using a USB Keyboard](#) on page 80

Using Flatness Correction

User flatness correction allows the digital adjustment of RF output amplitude for up to 1601 sequential linearly or arbitrarily spaced frequency points to compensate for external losses in cables, switches, or other devices. Using an Agilent N1911A/12A, E4419A/B, or U2000 Series power meter/sensor to calibrate the measurement system, a table of power level corrections can automatically be created for frequencies where power level variations or losses occur. Supported connection types to the power meter/sensor are Sockets LAN, VXI-11 LAN, USB, and GPIB via VXI-11 LAN using a LAN-GPIB gateway (e.g. E5810A Gateway or equivalent).

NOTE A power meter with GPIB requires using the Connection Type **VXI-11** softkey, as well as a LAN-GPIB gateway, to control a power meter. Refer to the Agilent Connectivity Guide USB/LAN/GPIB Connectivity Guide (E2094-90009), Agilent MXG's FAQs "How do I connect to the LAN?", and to the E5810A User's Guide or equivalent, LAN/GPIB gateway device.

If you do not have an Agilent N1911A/12A or E4419A/B power meter, or U2000A/01A/02A/04A power sensor, or if your power meter does not have a LAN, GPIB, or USB interface, the correction values can be manually entered into the signal generator.


To allow different correction arrays for different test setups or different frequency ranges, you may save individual user flatness correction tables to the signal generator's memory catalog and recall them on demand.

Follow the steps in the next sections to create and apply user flatness correction to the signal generator's RF output (see [page 62](#)).

Afterward, follow the steps in "Recalling and Applying a User Flatness Correction Array" on [page 66](#) to recall a user flatness file from the memory catalog and apply it to the signal generator's RF output.

Figure 4-1 User Flatness Correction Softkeys

For details on each key, use key help as described on see [page 26](#).

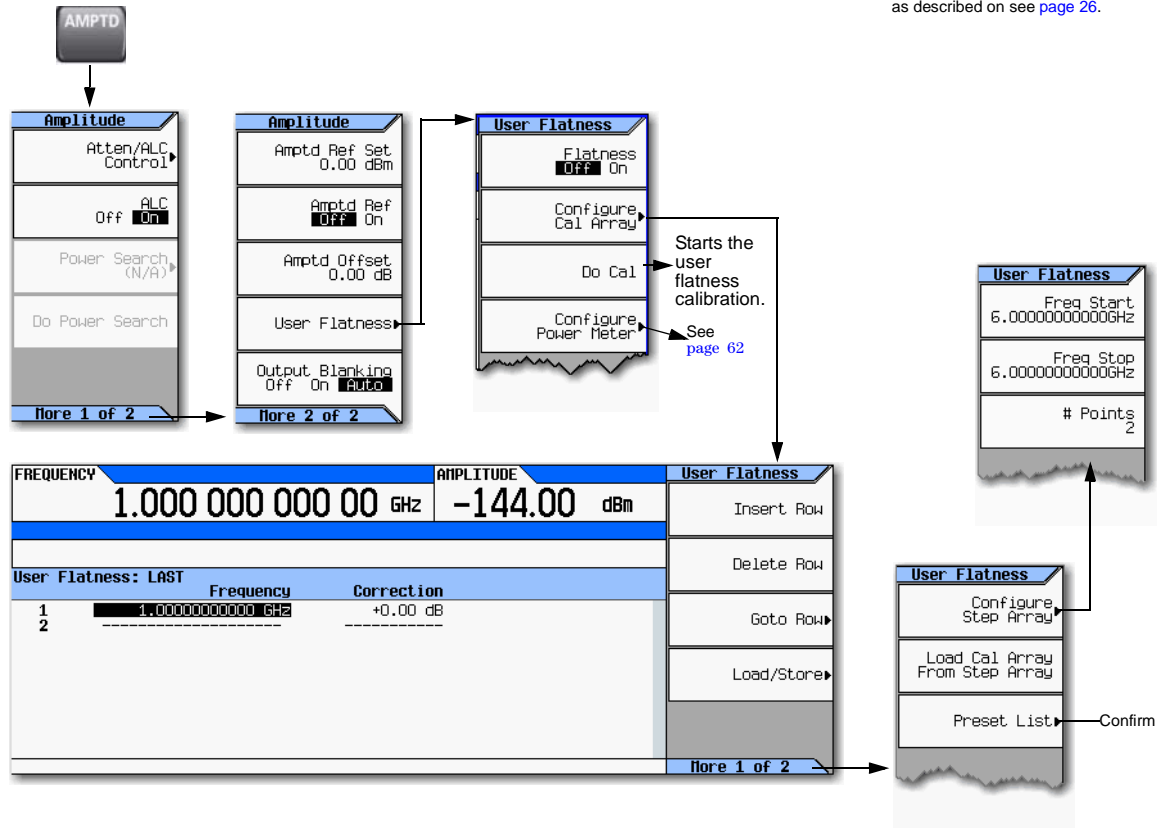

Creating a User Flatness Correction Array

In this example, you will create a user flatness correction array. The flatness correction array contains ten frequency correction pairs (amplitude correction values for each specified frequency), from 500 MHz to 1 GHz.

An Agilent N1911A/12A or E4419A/B power meter and E4413A power sensor are used to measure the RF output amplitude at the specified correction frequencies and transfer the results to the signal generator. (A U2000 Series power meter/sensor could be used in lieu of the power meter and E4413A power sensor.) The signal generator reads the power level data from the power meter, calculates the correction values, and stores the correction pairs in the user flatness correction array.

If you do not have the required Agilent power meter, or if your power meter does not have a LAN, GPIB, or USB interface, you can enter correction values manually.

NOTE On the N5183A, if the setup is using an external leveling configuration, the equipment setup in [“Required Equipment” on page 60](#) assumes that the steps necessary to correctly level the RF output have been followed. If you have questions about external leveling, refer to [“Using External Leveling” on page 67](#).

Required Equipment

- Agilent N1911A/12A or E4419A/B power meter (a power meter is *not* required with the U2000A/01A/02A/04A Power Sensor)
- Agilent E4413A E Series CW power sensor or U2000A/01A/02A/04A Power Sensor
- GPIB, LAN, or USB interface cables, as required
- adapters and cables, as required

NOTE For operating information on a particular power meter/sensor, refer to its operating guide.


Connect the Equipment

Connect the equipment as shown in [“Connect the Equipment” on page 61](#).

NOTE During the process of creating the user flatness correction array, the power meter is remotely controlled by the signal generator.


Connect the Equipment

- Agilent N1911A/12A or E4419A/B power meter^a
- Agilent U2000A/01A/02A/04A power Sensor^a
- LAN, GPIB, or USB interface cables, as required
- adapters and cables, as required

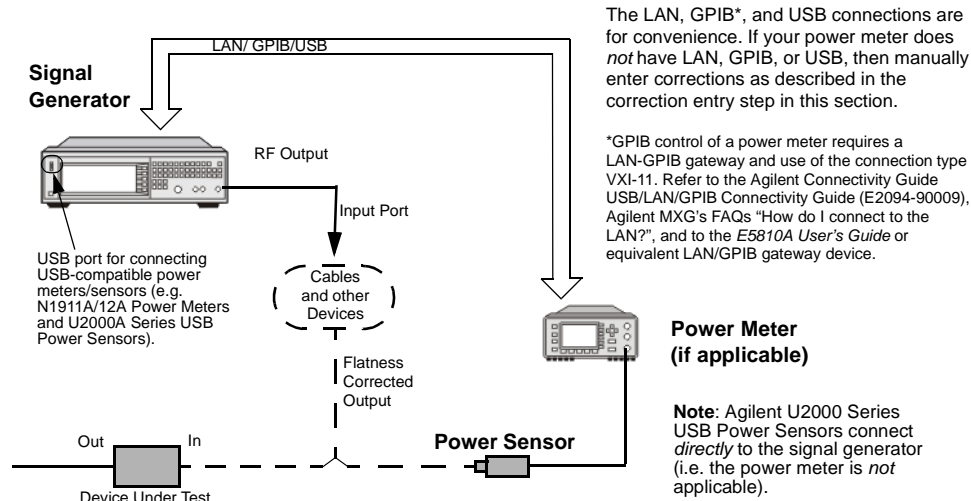

^aFor operating information, refer to the power meter/sensor documentation.

Figure 4-2 Configure Power Meter Menu Softkeys

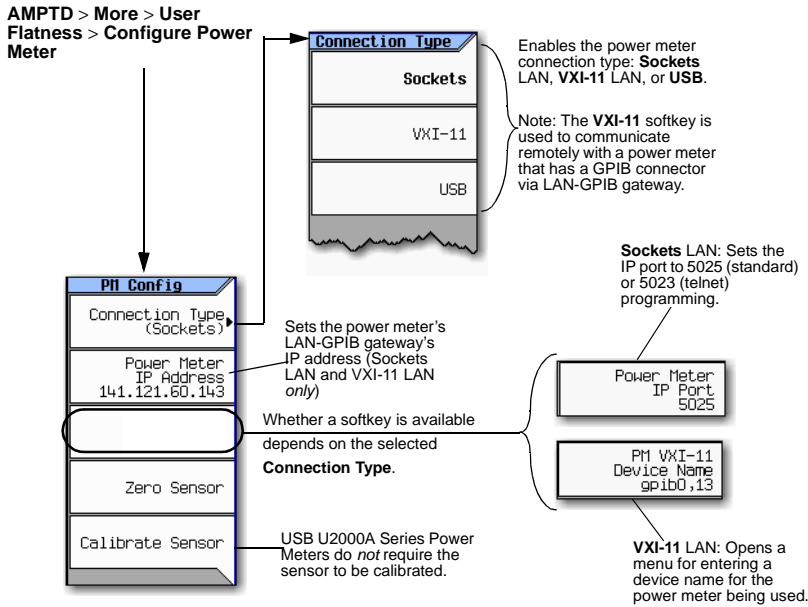

Basic Procedure

1. Create a user flatness array.
 - a. Configure the power meter/sensor
 - b. Connect the equipment
 - c. Configure the signal generator
 - d. Enter the user flatness correction values
2. Optionally, save the user flatness correction data.
3. Apply user flatness correction to the RF Output.

Configure the U2000A/01A/02A/04A Power Sensor

1. Connect to the signal generator's front panel USB port. Refer to [“Connect the Equipment” on page 61](#).
2. Zero the power sensor using the signal generator.

CAUTION Verify the signal generator RF Output power is set to the desired amplitude before performing the power meter zero. *No RF Output amplitude check is done by the signal generator during zero.*

NOTE The signal generator's RF Output LED remains unchanged during zeroing of the power sensor (e.g. if the RF Output LED was on prior to starting the Zeroing of the power sensor, the LED remains on throughout the zero/calibration). But, actually the instrument's firmware has turned *off* the RF Output's power.

For operating information on your particular power sensor, refer to its operation guide.

Configure the E4419A/B and N1911A/12A Power Meter

1. Select SCPI as the remote language for the power meter.
2. Zero and calibrate the power sensor to the power meter, using the softkeys on the signal generator *or* the front panel of the power meter.
3. Enter the power sensor calibration factors into the power meter as required.
4. Enable the power meter's cal factor array.

NOTE The signal generator's RF Output LED remains unchanged during zeroing of the power sensor (e.g. if the RF Output LED was on prior to starting the Zeroing of the power sensor, the LED remains on throughout the zero/calibration). But, actually the instrument's firmware has turned *off* the RF Output's power.

For operating information on your particular power meter/sensor, refer to its operating guide.

Example: A 500 MHz to 1 GHz Flatness Correction Array with 10 Correction Values

Create the User Flatness Array

1. Configure the signal generator:
 - a. Preset the signal generator.
 - b. Set the signal generator's connection type to the power meter/sensor:
 - i. Press **AMPTD** > **More** > **User Flatness** > **Configure Power Meter** > **Connection Type** > *connection type*.
 - ii. If connection type is USB:
 1. Zero Sensor
 2. Go to step **c**.

else

If Sockets LAN or VXI-11 LAN: Press **Power Meter IP Address** > *power meter's or LAN-GPIB gateway IP address* > **Enter**.

- iii. If Sockets LAN: Press **Power Meter IP Port** > *IP port* > **Enter**.

else

If VXI-11: Press **PM VXI-11 Device Name** > *device name* > **Enter**.

When connecting directly to the power meter, enter the *device name* as specified in the power meter's documentation. Typically, this is "inst0" and is case sensitive for some power meters. Refer to your power meter's documentation, the Agilent Connectivity Guide USB/LAN/GPIB Connectivity Guide (E2094-90009), and Agilent MXG's FAQs "How do I connect to the LAN?"

When connecting via a LAN-GPIB gateway, enter the SICL address of the power meter. Typically, this is "gpib0,13", where "gpib0" is the GPIB SICL interface name of the gateway and "13" is the GPIB address of the power meter. Refer to the Agilent Connectivity Guide USB/LAN/GPIB Connectivity Guide (E2094-90009), Agilent MXG's FAQs "How do I connect to the LAN?", and to the E5810A User's Guide or equivalent, LAN/GPIB gateway device.

- c. Open the User Flatness table editor and preset the cal array:
Press **Return** > **Configure Cal Array** > **More** > **Preset List** > **Confirm Preset with Defaults**.
- d. In the Step Array menu, enter the desired flatness-corrected start and stop frequencies, and the number of points:

Press **More** > **Configure Step Array** >

Freq Start > **500** > **MHz** >

Freq Stop > **1** > **GHz** >

of Points > **10** > **Enter**

- e. Populate the user flatness correction array with the step array configured in the previous step:

Press **Return** > **Load Cal Array From Step Array** > **Confirm Load From Step Data**.

- f. Set the output amplitude to 0 dBm.
- g. Turn on the RF output.

2. Connect the power meter to the RF output and enter the correction values:

With a Power Meter Over LAN, GPIB, or USB	Manually
<p>i. Create the correction values: Press More > User Flatness > Do Cal.</p> <p>The signal generator begins the user flatness calibration, and displays a progress bar.</p> <p>The amplitude correction values load automatically into the user flatness correction array.</p> <p>ii. View the stored amplitude correction values: Press Configure Cal Array.</p>	<p>i. Open the User Flatness table editor and highlight the frequency value in row 1: Press More > User Flatness > Configure Cal Array.</p> <p>The RF output changes to the frequency value of the table row containing the cursor.</p> <p>ii. Note the value measured by the power meter.</p> <p>iii. Change the sign on the delta value (e.g. <i>the delta value of the 0 dBm reference value (step f), and the measured value from ii is -.34, change the value to +.34</i>).</p> <p>iv. Highlight the correction value in row 1.</p> <p>v. Press Select > enter the delta calculated in step iii > dB. (e.g. For this example enter +.34) The signal generator adjusts the output amplitude based on the correction value entered.</p> <p>vi. Repeat steps ii – v until the power meter reads 0 dBm.</p> <p>vii. Highlight the frequency value in the next row.</p> <p>viii. Repeat steps ii through vii for the remaining rows.</p>

The user flatness correction array title displays `User Flatness: (UNSTORED)`, without a name, indicating that the current user flatness correction array data has *not* been saved to the file catalog.

Optional: Save the User Flatness Correction Data

1. Press **Load/Store > Store to File.**

2. Enter a file name (for this example, `FLATCAL1`) and press **Enter.**

The user flatness correction array file is now stored in the file catalog as a `USERFLAT` file. Any user flatness correction files saved to the catalog can be recalled, loaded into the correction array, and applied to the RF output to satisfy specific RF output flatness requirements.

3. Press **Return.**

Enable the Flatness Correction at the RF Output

- Press **Return > Flatness Off On.**


The UF annunciator appears in the `AMPLITUDE` area of the display, and the correction data in the array is applied to the RF output.

Recalling and Applying a User Flatness Correction Array

The following example assumes that a user flatness correction array has been created and stored. If not, perform the [Example: A 500 MHz to 1 GHz Flatness Correction Array with 10 Correction Values](#) on page 63.


1. Preset the signal generator.
2. Recall the desired User Flatness Correction file:
 - a. Press **AMPTD > More > User Flatness > Configure Cal Array > More > Preset List > Confirm Preset.**
 - b. Press **More > Load/Store.**
 - c. Highlight the desired file.
 - d. Populate the user flatness correction array with the data contained in the selected file:
Press **Load From Selected File > Confirm Load From File.**
The user flatness correction array title displays User Flatness: *Name of File.*
3. Apply the correction data in the array to the RF output: Press **Return > Flatness Off On to On.**

Using External Leveling

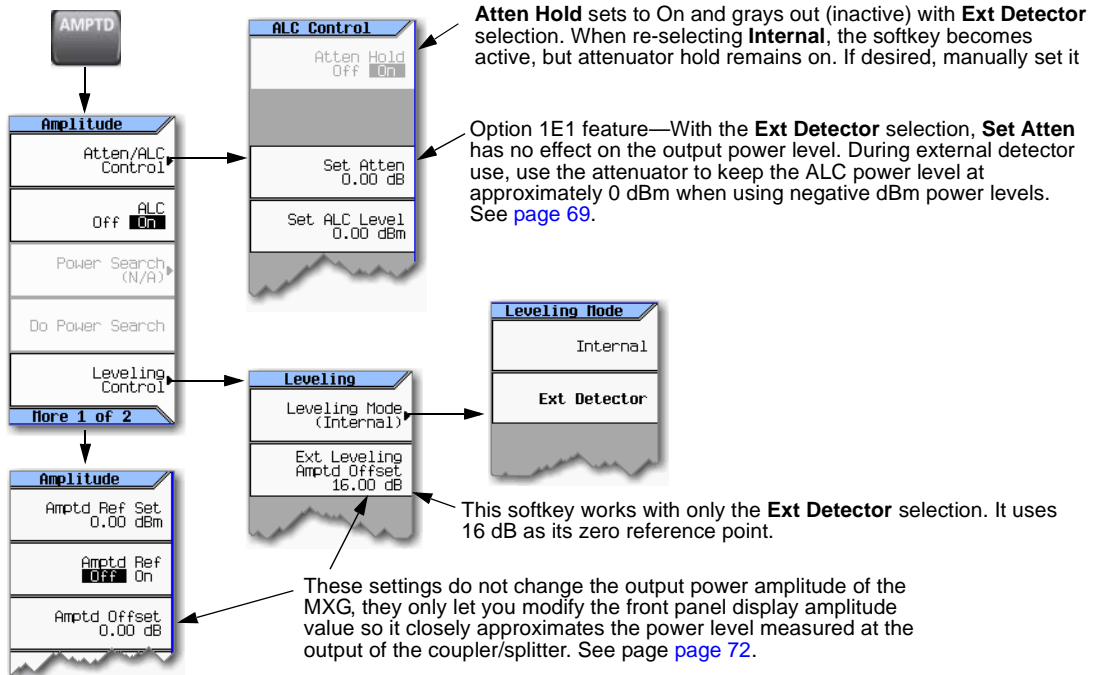

External leveling lets you move the ALC feedback source closer to the device under test (DUT) so that it accounts for most of the power uncertainties inherent to the cabling and components in a test setup. Refer to [Figure 4-3](#).

Figure 4-3 ALC Circuitry

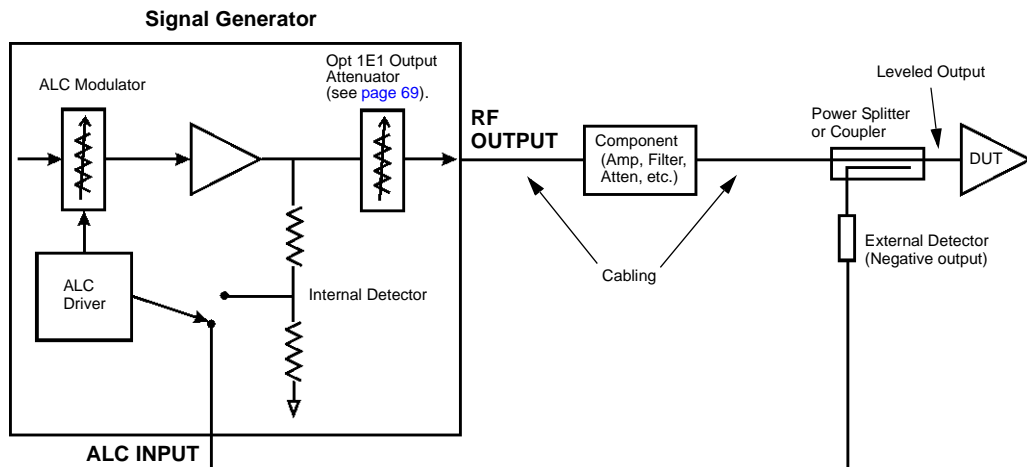

The external detector outputs a negative voltage to the signal generator's rear-panel ALC INPUT connector based on the power level at the detector. As the RF power level at the coupler's/power splitter input changes, the external detector returns a compensating negative voltage. The ALC circuit uses this negative voltage to level the RF output power by raising and lowering the signal's power, thus ensuring a constant power level at the point of detection (external detector). Since the point of detection does not occur at the output of the device to which the detector is connected, there is some power loss that is not compensated for by the external detector. For example on a coupler, the coupled port siphons some of the signal's energy to drive the external detector. In addition the coupler experiences some insertion loss between the coupled port and the output.

Figure 4-5 on page 69 shows the input power versus output voltage characteristics for typical Agilent Technologies diode detectors. Using this chart, you can determine the leveled power at the diode detector input by measuring the external detector output voltage. For a coupler, you must then add the coupling factor to determine the leveled output power.

When using an external detector, the signal generator's power range may vary from the values shown in the data sheet. This is primarily due to the efficiency of the detector. Always ensure that the detector, coupler/power splitter are specified for the power and frequency range of interest. To determine the signal generator's actual power range during external leveling, see "Determining the Signal Generator's Amplitude Range" on page 71.

With external leveling, the displayed amplitude value can vary significantly from the actual output power of the coupler/power splitter to which the external detector is connected (see Figure 4-4). This is because the coupler/power splitter has its own signal characteristics (insertion loss, coupling factor, and so forth), which are unknown to the signal generator, so it is typically unable to display an accurate amplitude value. Also components between the signal generator and the external detector can affect the output power of the coupler/power splitter. You can compensate for this power display difference by using the

Ext Leveling Amptd Offset softkey or the **Amptd Offset** softkey. The difference between the two softkeys is that the **Ext Leveling Amptd Offset** functions only while external leveling is active. For more information on using the external leveling offset feature, see "Adjusting the Signal Generator Display's Amplitude Value" on page 72.

Figure 4-4 Power Value Differences with External Leveling


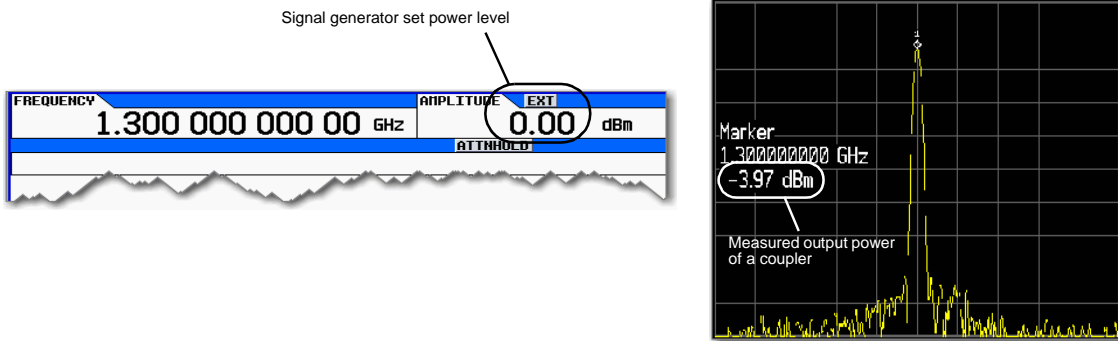


Figure 4-5 Typical Diode Detector Response at 25° C

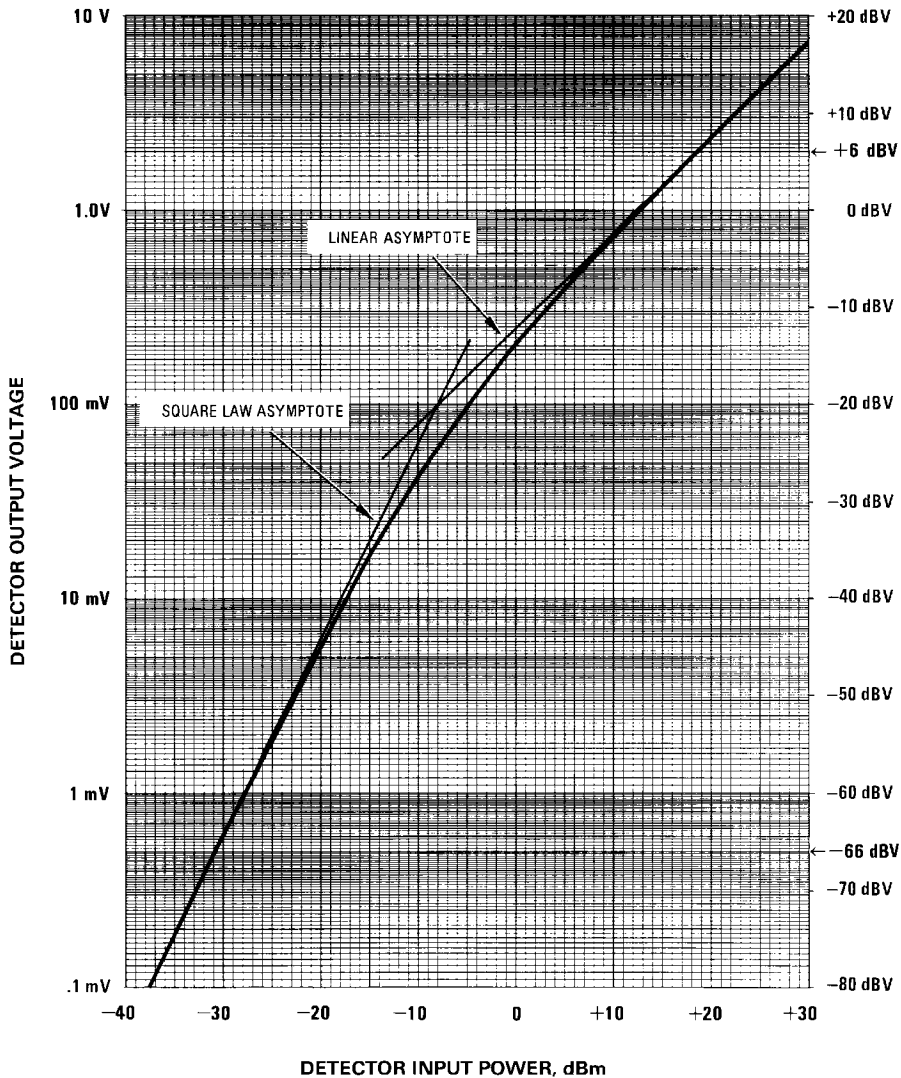

Option 1E1 Output Attenuator Behavior and Use

When using the internal detector, the Option 1E1 output attenuator enables signal generator power levels down to -135 dBm at the RF Output connector. It accomplishes this by adding attenuation to the output signal after the ALC detection circuit. The output power value (shown in the Amplitude area of the display) is the resultant of the **Set Atten** and **Set ALC Level** values (see [page 67](#)). With the external detector selected, the output attenuator no longer attenuates the output signal since the

feedback for the detection circuit has been moved beyond the output attenuator. Because the attenuator no longer affects the amplitude of the output signal, the output amplitude is determined by only the **Set ALC Level** softkey.

With external leveling selected, the signal generator enables attenuator hold and the power range approximates the range of a standard option (no attenuator) signal generator (see the *Data Sheet*). As stated earlier, the actual output power may vary due to the external detector and the coupler/power splitter performance characteristics.

NOTE When the internal detector (**Internal** selection) is reselected, the signal generator does not turn the attenuator hold off.

Even though the output attenuator no longer affects the output power, it is still useful to drive the ALC circuit to its mid-power point of approximately 0 dBm, which is optimal for the internal leveling circuitry and typically provides the best amplitude flatness results. This is useful with negative power values of -5 dBm or less. For example, to drive the ALC to approximately mid-power with a -20 dBm power setting, add 25 dB of attenuation. This sets the ALC circuit to 5 dBm (-20 + 25).

NOTE If there is too much attenuation, it will drive the ALC circuit too high and cause the signal generator to go unlevelled. Ensure that you decrease the attenuation as you increase the power level.

Configure External Leveling

Basic Setup Process

- If working with a single frequency signal, perform Steps 1 through 5.
 - If working with multiple frequencies:
 - a. Perform Steps 1 through 4.
 - b. Perform a user flatness correction, see [“Using Flatness Correction” on page 58](#).
 - If working with a sweep:
 - a. Perform Steps 1 through 4.
 - b. Setup the sweep, see [“Configuring a Swept Output” on page 31](#).
1. Setup the equipment, see [“Equipment Setup” on page 70](#)
 2. Configure the carrier signal, see [“Configuring the Carrier” on page 71](#)
 3. Select external leveling, see [“Selecting External Leveling” on page 71](#).
 4. Determine the output amplitude range, see [“Determining the Signal Generator’s Amplitude Range” on page 71](#)
 5. Set the displayed power value, see [“Adjusting the Signal Generator Display’s Amplitude Value” on page 72](#)


Equipment Setup

Set up the equipment as shown in [Figure 4-6 on page 71](#). Place the external detector (detector and coupler/power splitter) as close as possible to the DUT.

Recommended Equipment

- Agilent 8474E negative detector
- Agilent 87301D directional coupler
- cables and adapters, as required

Figure 4-6 Typical External Leveling Setup using a Directional Coupler

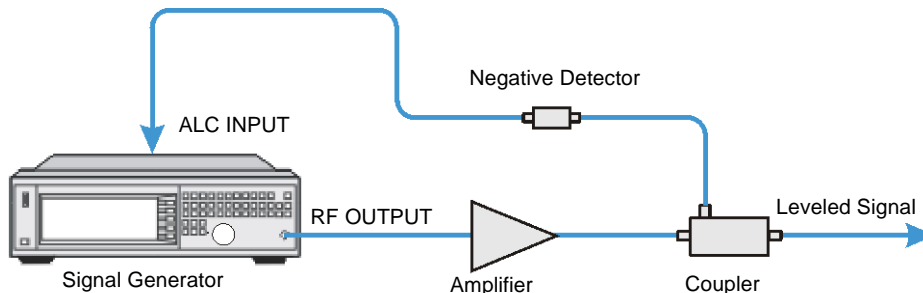

Configuring the Carrier

1. Press **Preset**.
2. Set the carrier frequency.
3. Set the power level to 0 dBm:
 - If the signal generator has no output attenuator (no Option 1E1) or it has Options 1E1 and 532 or 540 installed:
Press **AMPTD > 0 > dBm**.
 - If the signal generator has Options 1E1 and 520, set the output attenuator to zero dBm:
 - a. Press **AMPTD > Atten/ALC Control > Atten Hold Off On** to On.
 - b. Press **Set Atten > 0 > dB**.
 - c. Press **Set ALC Level > 0 > dBm**.

Selecting External Leveling

Press **AMPTD > Leveling Control > Leveling Mode > Ext Detector**.

Determining the Signal Generator's Amplitude Range

The maximum output amplitude is frequency dependent. So if you are using multiple frequency points and there is a need to know the maximum output amplitude for each frequency point, refer to the *Data Sheet* for the power bands. Then use this procedure to determine the maximum amplitude for each band.

With external leveling and Option 1E1, the signal generator's the power range approximates that of a standard option instrument (no Option 1E1). But Option 1E1 does let you use the attenuator to drive the ALC to its mid-power point when using negative amplitude values. However adding attenuation does decrease the upper range limit. For more information, see ["Option 1E1 Output Attenuator"](#)

Behavior and Use” on page 69.

1. If Option 1E1 is installed, adjust the attenuator to the desired level.

NOTE If the Option 1E1 output attenuator value is too high (approximately ≥ 55 dB), it will cause an unlevel condition to occur when the RF output is turned on.

- a. Press **AMPTD > Atten/ALC Control > Set Atten.**
 - b. Enter the attenuator value.
2. Turn on the RF output: Press **RF On/Off** to On
 3. Set the **AMPTD** step increment value to one dB.
 - Press **AMPTD > Incr Set > 1 > dB.**
 4. Determine the minimum amplitude value:
 - a. Set the amplitude to -25 dBm.
 - b. Using the down arrow key, decrease the amplitude until the UNLEVEL annunciator appears.
 - c. Using the up arrow key, increase the amplitude until the UNLEVEL annunciator is gone.
The value showing when the UNLEVEL annunciator is gone is the minimum amplitude range value.
 5. Determine the maximum amplitude value:
 - a. Set the amplitude to a value that does not cause the signal generator to go unlevelled.
 - b. Using the up arrow key, increase the amplitude until it goes unlevelled or an error message indicating that the upper limit has been reached shows at the bottom of the display.
 - c. Decrease the amplitude value:
 - If the unlevelled annunciator appeared, decrease the amplitude until the annunciator is gone. The value where the annunciator disappears is the maximum upper range value.
 - If the signal generator displays Error: 501, Attenuator hold setting over range at the bottom of the display, the value showing is the maximum upper range value.
To remove the error message, press the down arrow key until the message is gone. The error appears when an attempt is made to increase the amplitude beyond the maximum value as it relates to the current attenuator setting.

Adjusting the Signal Generator Display's Amplitude Value

When using external leveling, the signal generator's displayed amplitude value will not match the leveled power of the signal at the output of the coupler/splitter. To compensate for this difference, the signal generator provides two methods for configuring the displayed power value so that it closely matches the measured value at the output of the coupler/splitter.

1. Connect and configure a measurement instrument:
 - a. Connect the output of the coupler/splitter to either a power meter or a signal analyzer.
 - b. Configure the power meter/signal analyzer for measuring the power level of the signal.
2. Adjust the signal generator's displayed amplitude value:

- If using the **Ext Leveling Amptd Offset** Softkey:


This softkey uses 16 dB as its zero reference. The 16dB is the coupling factor of the internal detector.

 - On the signal generator, press **AMPTD > Leveling Control > Ext Leveling Amptd Offset**.
 - While viewing the carrier amplitude value on the signal generator display, use the RPG knob (detent knob) to adjust the offset value until the integer part of the displayed amplitude value is the same as the integer portion of the measured value.

Each detent position adjusts the value by 1 dB.
 - Using the number keypad, make the necessary fractional adjustments to the display amplitude value.
- If using the **Amptd Offset** Softkey:
 - On the signal generator, press **AMPTD > Leveling Control > More > Amptd Offset**.
 - Calculate the difference between the signal generators displayed Amplitude value and the measured value.
 - Using the numeric keypad, enter this difference as the **Amptd Offset** softkey value.

Using Unleveled Operating Modes

Figure 4-7 Power Search and ALC Off Softkeys

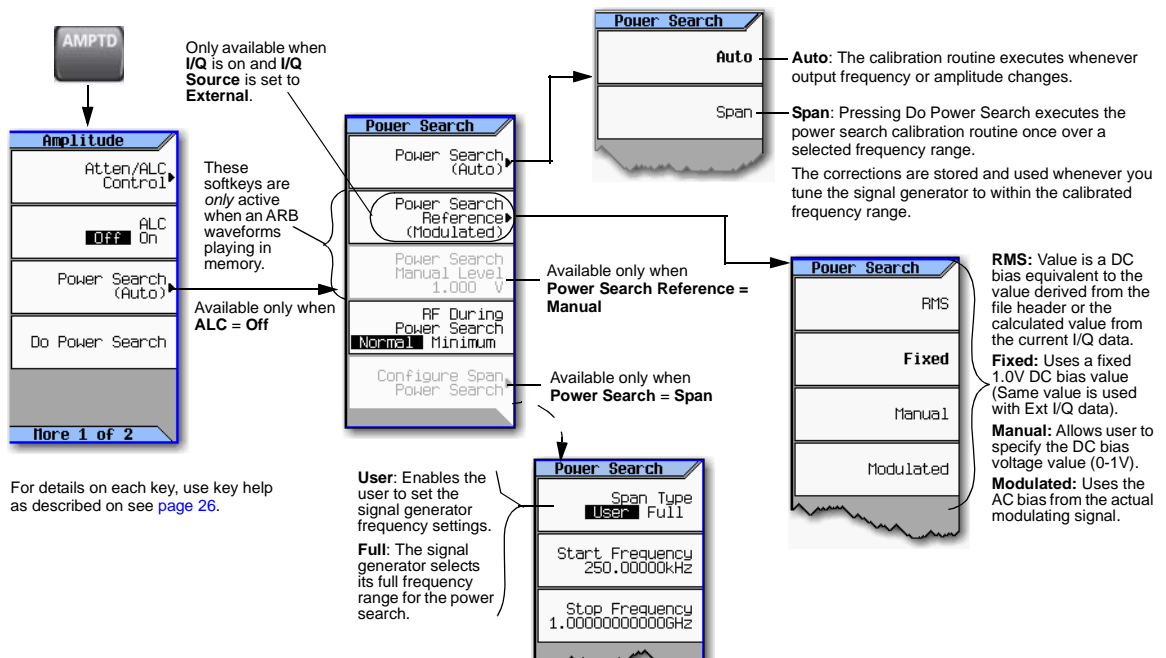

ALC Off Mode

Turning ALC off deactivates the signal generator's automatic leveling circuitry, enabling you to measure the output at a specific point in a test setup and adjust as required for the desired power level at that point. Turning ALC off is useful when the modulation consists of very narrow pulses that are below the pulse width specification of the ALC or when the modulation consists of slow amplitude variations that the automatic leveling would remove.

1. Preset the signal generator.
2. Set the desired frequency.
3. Set the desired amplitude.
4. Connect the power meter to the point at which you want a specific power level.
5. Turn the RF output on.
6. Deactivate the signal generator's automatic leveling control: Press **AMPTD > ALC Off On** to highlight Off.
7. Adjust the signal generator's amplitude until the power meter measures the desired level.

Power Search Mode

Refer to [Figure 4-7 on page 73](#). Power search executes a routine that temporarily activates the ALC, calibrates the power of the current RF output, and then disconnects the ALC circuitry.

NOTE For the power search routine to execute, RF must be on and ALC must be off.

Example: Automatic Power Search

1. Preset the signal generator.
2. Set the desired frequency.
3. Set the desired amplitude.
4. Turn the RF output on.
5. Deactivate the signal generator's automatic leveling control:

Press **AMPTD > ALC Off On** to highlight Off

Deactivating the signal generator's automatic leveling control is a significant instrument change that automatically initiates a power search.

When set to Auto, power search automatically executes when a significant instrument setting changes. The Do Power Search feature enables you decide when to execute a power search to compensate for changes, such as temperature drift or a change in the external input.

Using an Output Offset, Reference, or Multiplier

Setting an Output Offset


Using an output offset, the signal generator can output a frequency or amplitude that is offset (positive or negative) *from* the entered value.

RF Output = entered value – offset value

Displayed Value = output frequency + offset value

To set an offset:


- *Frequency:* Press **Freq** > **Freq Offset** > *offset value* > *frequency unit*.
- *Amplitude:* Press **Amptd** > **More** > **Amptd Offset** > *offset value* > **dB**.

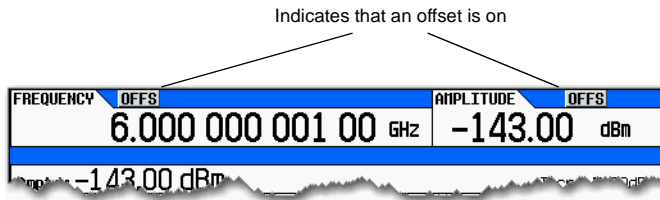

Examples

Parameter	Example #1	Example #2	Example #3	Comments
Entered (and displayed) Value:	300 MHz	300 MHz	2 GHz	The entered value must be positive.
Offset:	50 MHz	-50 MHz	-1 GHz	An offset value can be positive or negative.
Output Frequency:	250 MHz	350 MHz	3 GHz	The signal generator alerts you if the output frequency or amplitude is out of range.

When using the signal generator as a local oscillator (LO), you can use the offset to display the frequency of interest, as illustrated below:

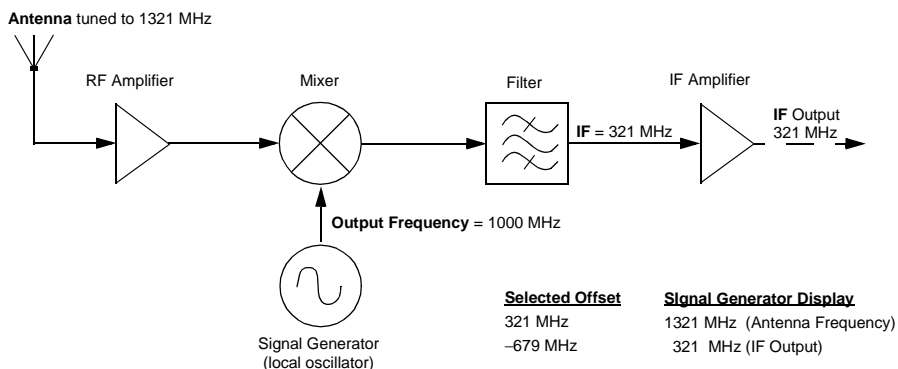


Setting an Output Reference

Using an output reference, the signal generator can output a frequency or amplitude that is offset (positive or negative) *by* the entered value *from* a chosen reference value.

RF Output = reference value + entered value

To set a reference:

1. Set the frequency or amplitude to the value you want as the output reference level.
2. *Frequency:* Press **Frequency > Freq Ref Set**
The frequency displays 0.00 Hz, indicating that this is the RF output frequency “zero level.” All frequencies entered are interpreted as being relative to this reference frequency.
Amplitude: Press **Amptd > More > Amptd Ref Set**
The amplitude displays 0.00 dB, indicating that this is the RF output amplitude “zero level.” All amplitudes entered are interpreted as being relative to this reference amplitude.

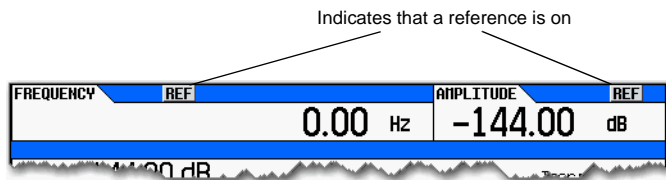

Examples

Parameter	Example #1	Example #2	Example #3	Comments
Reference:	50 MHz	50 MHz	2 GHz	A reference value must be positive.
Entered (and displayed) Value:	2 MHz	-2 MHz	-1 GHz	The entered value can be positive or negative.
Output Frequency:	52 MHz	48 MHz	1 GHz	The signal generator alerts you if the output frequency or amplitude is out of range.

To set a new frequency or amplitude reference, turn the frequency reference off, and then follow the steps above.

Setting a Frequency Multiplier

Using a frequency multiplier, the signal generator can display a frequency that is the multiple (positive or negative) of the output frequency.


Displayed Value = multiplier value × output frequency

Output Frequency = displayed value ÷ multiplier value

To set a frequency multiplier:

1. Press **Frequency** > **Freq Multiplier** > *multiplier value* > **x**.
2. Set the desired frequency.
The display equals the output frequency times the multiplier value.


Indicates that a frequency multiplier is on

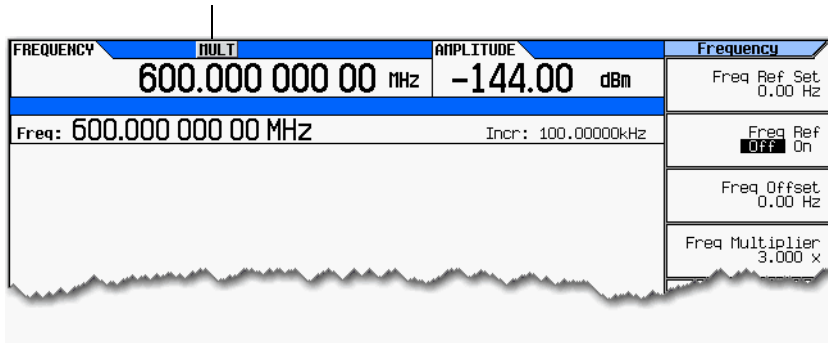


Examples

Parameter	Example #1	Example #2	Example #3	Comments
Frequency Multiplier:	3	-3	4	A multiplier value can be positive or negative.
Entered (and displayed) Value:	600 MHz	-600 MHz	8 GHz	
Output Frequency:	200 MHz	200 MHz	2 GHz	The signal generator alerts you if the output frequency is out of range.

When using the signal generator as the input to a system, you can set the frequency multiplier so that the signal generator displays the output of the system, as illustrated below using a doubler:

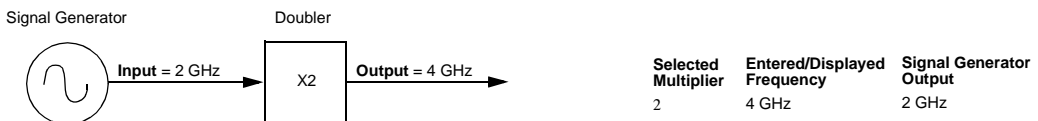

When measuring mixers, the frequency multiplier and frequency offset are often used together. In the upconverter example below, the multiplier is set to -1 and the offset is set to 3 GHz so that the signal generator displays f_{RF} .

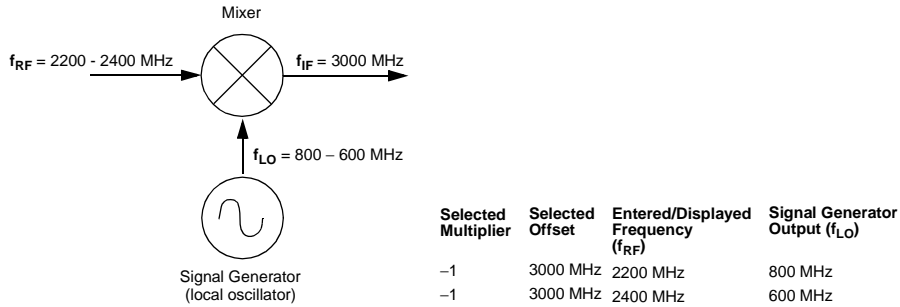

Using Free Run, Step Dwell, and Timer Trigger

Free Run, Step Dwell (time), and Timer Trigger can be used to adjust the time spent at any point in a Step Sweep or a List Sweep. There are two possible measurement combinations:

Free Run with Step Dwell time (Figure 4-8 on page 79) the signal generator waits for the signal to settle and then waits for the Step Dwell time, then it jumps to the next frequency point. In addition, the time to complete the entire sweep can vary. There is *always* a minimum value of Step Dwell for each frequency point. The minimum Step Dwell timing for any point is fixed at a value of 100 μ s. The time between frequency points is the sum of the settling time, plus the Step Dwell time. The settling time is dependent on frequency, amplitude, band crossings, and other factors, so the time between frequency points can vary.

Timer Trigger instead of Free Run (Figure 4-8 on page 79) the signal generator generates equally spaced triggers, and it moves to the next point at each trigger. This has the advantage that the time between points is consistent and the overall sweep time is consistent. But, if the trigger is too fast, the signal may not have time to settle before jumping to the next point.

Understanding Free Run, Step Dwell, and Timer Trigger Setup


If the signal is to be settled for a minimum specific time at each point and it is *not* important if the point-to-point time is consistent, use **Free Run** and **Set Dwell** time.

If the signal's point-to-point time requires consistency but the specific settling time at each point can vary, then use the Timer Trigger. Avoid using too fast of a sweep which does *not* allow the signal generator to settle.

If the signal needs to be settled for a specific minimum time *and* consistent point-to-point time is required, then you should set the Timer Trigger to be the sum of the switching time (900 μ s or 5 ms, depending on options) *plus* the minimum settled time that is needed to make the measurement.

If the measurement requires external equipment synchronization, consider using hardware triggers.

Figure 4-8 Free Run, Set Dwell, and Timer Trigger Softkeys

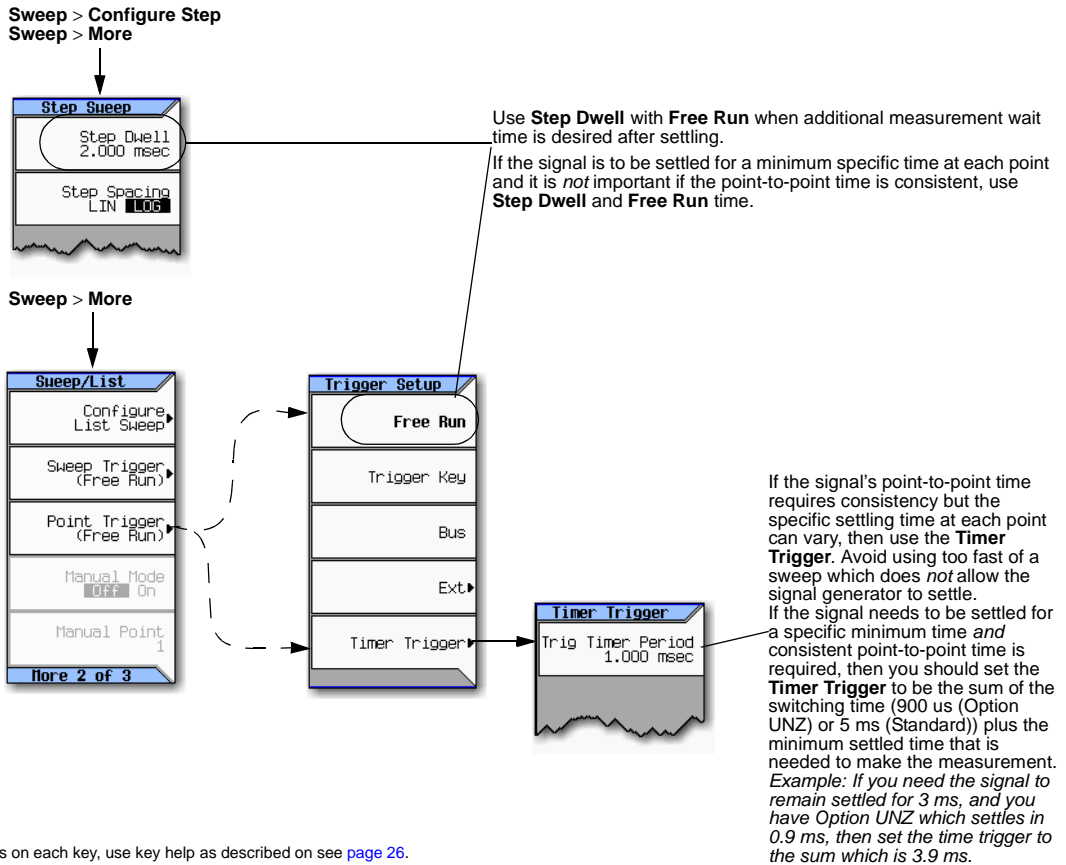

For details on each key, use key help as described on see [page 26](#).

Using a USB Keyboard

You can use a USB keyboard to remotely control the RF output state, the modulation state, and to select a memory sequence and register.

The register selection, RF output state, and modulation state are affected by power cycle or preset, but the USB keyboard control state and the sequence selection are not.

USB Keyboard Key	Signal Generator Function
Delete, Enter	RF On/Off
Insert	Mod On/Off
Home, Up Arrow	Next Sequence
End, Down Arrow	Previous Sequence
Page Up, Right Arrow, +	Recall Next State Register
Page Down, Left Arrow, -	Recall Previous State Register

Turning the USB keyboard control off disables the USB keyboard; it has no effect on the Auto Recall softkeys.


For details on each key, use key help as described on see [page 26](#).

5 Using Analog Modulation (Option UNT Only)

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting the power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

- [The Basic Procedure on page 82](#)
- [Using an External Modulation Source on page 83](#)
- [Removing a DC Offset on page 83](#)

Figure 5-1 Analog Modulation Softkeys

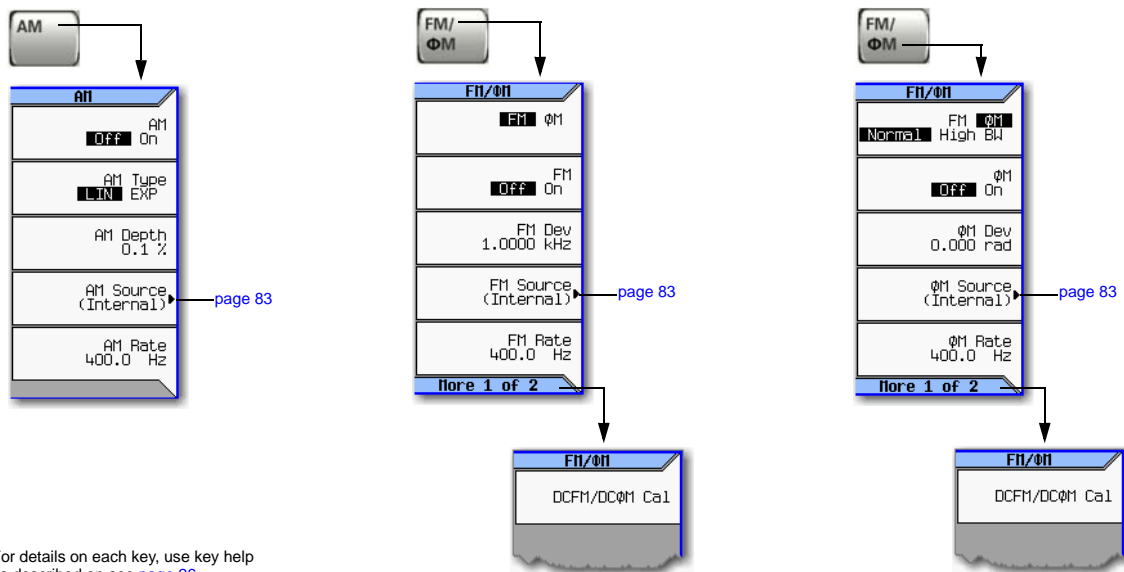

The Basic Procedure

1. Preset the signal generator.
2. Set the carrier (RF) frequency.
3. Set the RF amplitude.
4. Configure the modulation:

AM	FM	ΦM
a. Press AM b. Set the AM type (linear or exponential): AM Type to highlight desired type c. Set the depth: AM Depth > <i>value</i> d. Set the rate: AM Rate > <i>value</i> > <i>frequency unit</i>	a. Press FM/ΦM b. Set the deviation: FM Dev > <i>value</i> > <i>frequency unit</i> c. Set the rate: FM Rate > <i>value</i> > <i>frequency unit</i>	a. Press FM/ΦM > FM ΦM b. Set the BW (normal or high): FM ΦM to highlight desired type c. Set the deviation: ΦM Dev > <i>value</i> > pi rad d. Set the rate: ΦM Rate > <i>value</i> > <i>frequency unit</i>

5. Turn on the modulation:

AM	FM	ΦM
AM Off On softkey to On	FM Off On softkey to On	ΦM Off On softkey to On

The appropriate modulation annunciator displays, indicating that you enabled modulation.


6. Turn on the RF output.

The RF output LED lights, indicating that the signal is transmitting from the RF output connector.


If the modulation does not seem to be working properly, refer to [“No Modulation at the RF Output” on page 235](#).

See also [“Modulating the Carrier Signal” on page 43](#).

Using an External Modulation Source

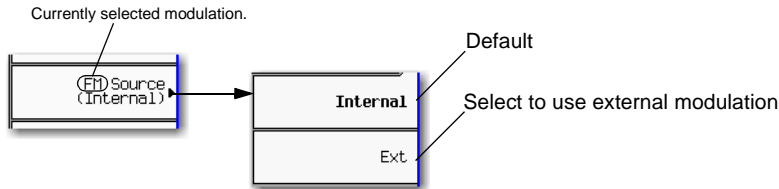

Rear panel inputs are described on [page 11](#)

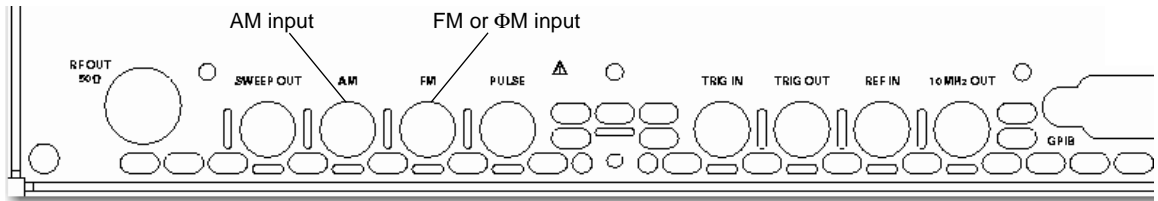

Removing a DC Offset

To eliminate an offset in an externally applied FM or Φ M signal, perform a DCFM or DC Φ M Calibration.

NOTE You can perform this calibration for internally generated signals, but DC offset is not usually a characteristic of an internally generated signal.

1. Set up and turn on the desired modulation.
2. Press **FM/ Φ M** > **More** > **DCFM/DC Φ M Cal.**


Performing the calibration with a DC signal applied removes any deviation caused by the DC signal, and the applied DC level becomes the new zero reference point. When you disconnect the DC signal, perform the calibration again to reset the carrier to the correct zero reference.

6 Using Pulse Modulation (Option UNU or UNW)

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting the power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

- [Pulse Characteristics](#) on page 87
- [The Basic Procedure](#) on page 89
- [Example](#) on page 89

Figure 6-1 Pulse Softkeys

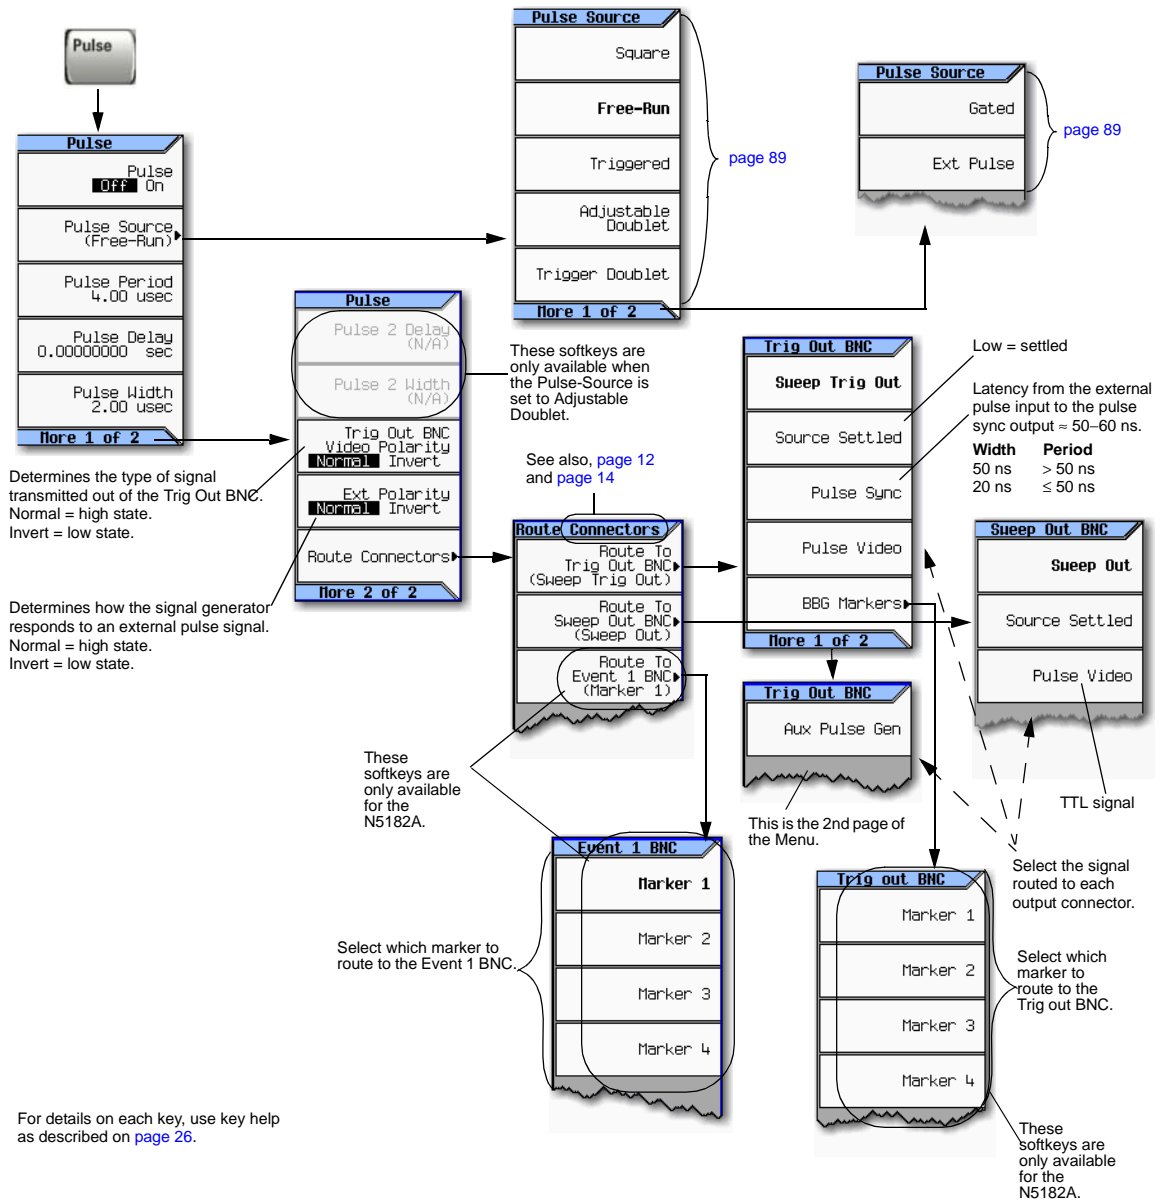

Pulse Characteristics

NOTE When using very narrow pulses that are below the signal generator's ALC pulse width specification, or leveled pulses with an unusually long duty cycle, it is often useful to turn ALC off (see [page 74](#)).

Pulse Source	Type	Period ^a	Width & Delay ^a	Uses Trigger Event ^b
Square	Internal free run pulse train with 50% duty cycle.	Determined by user defined rate.	—	—
Free Run (default)	Internal free run pulse train	User Defined	User Defined	—
Triggered	Internal pulse train	—	User Defined	✓
Adjustable Doublet	Two internal pulse trains for each trigger event.	—	User Defined: First pulse is relative to the rising edge of trigger signal. Second pulse is relative to the rising edge of first pulse. See Figure 6-2 on page 88	✓
Trigger Doublet	Two internal pulse trains for each trigger event.	—	The first pulse follows the trigger signal. Second pulse is user defined. See Figure 6-3 on page 88	✓
Gated	Internal gated pulse train	—	User Defined	✓
External	External pulse signal at the rear panel Pulse connector	—	—	—

^aAll delays, widths, and periods have a resolution of 10 ns.

^bA signal at the rear panel pulse connector must be held high for at least 20 ns to trigger an internally generated pulse.

Rear panel inputs are described on [page 11](#)

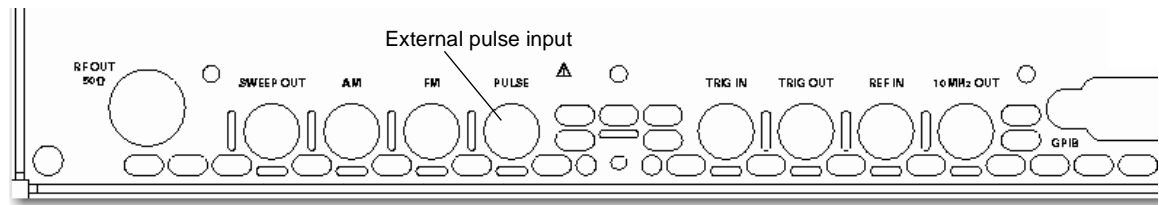


Figure 6-2 Adjustable Doublet


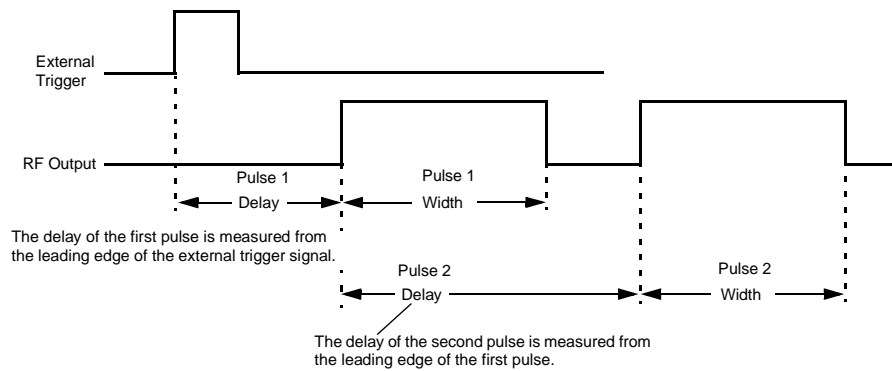


Figure 6-3 Trigger Doublet

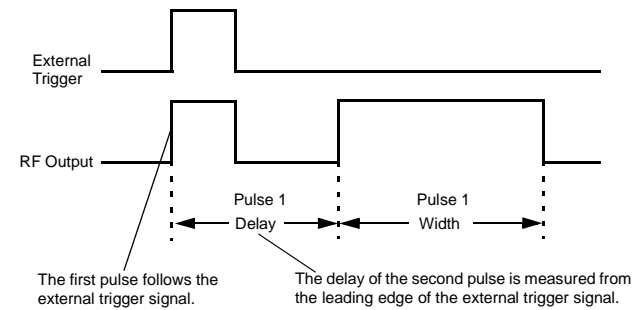

The Basic Procedure

1. Preset the signal generator.
2. Set the carrier (RF) frequency.
3. Set the RF amplitude.
4. Configure the modulation:
 - a. Set the pulse source: Press **Pulse > Pulse Source > selection**
 - b. Set the parameters for the selected pulse source:

Square	Free Run (default)	Triggered	Adjustable Doublet	Trigger Doublet	Gated	External
Pulse Rate	—	—	—	—	—	—
—	Pulse Period	—	—	—	Pulse Period	—
—	Pulse Delay	Pulse Delay	Pulse Delay	Pulse Delay	—	—
—	Pulse Width	Pulse Width	Pulse Width	Pulse Width	Pulse Width	—
—	—	—	Pulse 2 Delay	—	—	—
—	—	—	Pulse 2 Width	—	—	—

5. Turn on the modulation: **Pulse Off On** softkey to On.
The the PULSE annunciator lights, indicating that you enabled modulation.
6. Output the modulated signal from the signal generator: Press the front panel **RF On Off** key.
The RF output LED lights, indicating that the signal is transmitting from the RF output connector.
See also, [“Modulating the Carrier Signal” on page 43.](#)

Example

The following example uses the factory preset pulse source and delay.

Output: A 2 GHz, 0 dBm carrier modulated by a 24 μ s pulse that has a period of 100 μ s.

1. Preset the signal generator.
2. Set the frequency to 2 GHz.
3. Set the amplitude to 0 dBm.
4. Set the pulse period to 100 microseconds: Press **Pulse > Pulse Period > 100 > usec.**
5. Set the pulse width to 24 microseconds: Press **Pulse > Pulse Width > 24 > usec**
6. Turn on both the pulse modulation and the RF output.

The PULSE annunciator displays and the RF output LED lights.

If the modulation does not seem to be working properly, refer to [“No Modulation at the RF Output” on page 235.](#)

Using Pulse Modulation (Option UNU or UNW)
Example

7 Basic Digital Operation—No BBG Option Installed

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

See Also: [“Adding Real-Time Noise to a Dual ARB Waveform” on page 178](#)

I/Q Modulation


The following factors contribute to the error vector magnitude:

- Differences in amplitude, phase, and delay between the I and Q channels
- DC offsets

The I/Q menu provides adjustments to compensate for some of the differences in the I and Q signals or to add impairments.

See also, “Modulating the Carrier Signal” on page 43.

Figure 7-1 I/Q Display and Softkeys

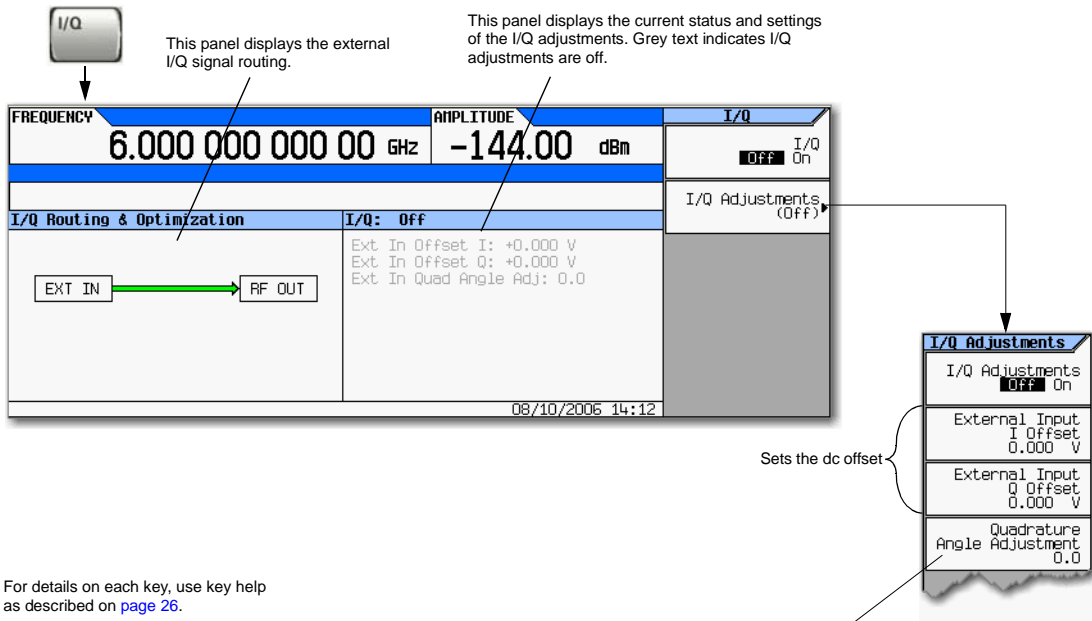

For details on each key, use key help as described on page 26.

The following table shows common uses for the adjustments.

Table 7-1 I/Q Adjustments Uses

I/Q Adjustment	Effect	Impairment
Offset	Carrier Feedthrough	dc offset
Quadrature Angle	EVM error	phase skew
	I/Q Images	I/Q path delay

Configuring the Front Panel Inputs

The Agilent MXG accepts externally supplied analog I and Q signals through the front-panel I Input and Q Input for modulating onto the carrier.

1. Connect I and Q signals to the front panel connectors. For voltage levels, refer to [“Front Panel Overview” on page 4](#).
 - a. Connect an analog I signal to the signal generator’s front-panel I Input.
 - b. Connect an analog Q signal to the signal generator’s front-panel Q Input.
2. Turn on the I/Q modulator: Press **I/Q Off On** to On.
3. Configure the RF output:
 - a. Set the carrier frequency.
 - b. Set the carrier amplitude.
 - c. Turn the RF output on.
4. Make adjustments to the I/Q signals ([page 92](#)) as needed.

8 Basic Digital Operation (Option 651/652/654)

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

The features described in this chapter are available only in vector signal generators with Option 651, 652, or 654.

- [Waveform File Basics](#) on page 96
- [Storing, Loading, and Playing a Waveform Segment](#) on page 98
- [Waveform Sequences](#) on page 101
- [Saving a Waveform’s Settings & Parameters](#) on page 105
- [Using Waveform Markers](#) on page 110
- [Triggering a Waveform](#) on page 126
- [Clipping a Waveform](#) on page 133
- [Scaling a Waveform](#) on page 142
- [Setting the Baseband Frequency Offset](#) on page 149
- [I/Q Modulation](#) on page 152
- [Multiple Baseband Generator Synchronization](#) on page 158
- [Waveform 5-Pack Licensing \(Options 221-229\)](#) on page 164

See Also:

- [“Adding Real-Time Noise to a Dual ARB Waveform” on page 178](#)
- [“Real-Time Phase Noise Impairment” on page 184](#)
- [Chapter 12, “Multitone and Two-Tone Waveform Generator \(Option 430\),” on page 213](#)

Waveform File Basics

There are two types of waveform files:

- A *segment* is a waveform file that you download to the signal generator.
For information on creating and downloading waveform files, refer to the *Programming Guide*.
- A *sequence* is a file you create in the signal generator that contains pointers to one or more waveform files (segments, other sequences, or both).
For information on creating sequences, see [page 101](#).

Signal Generator Memory

The signal generator has two types of memory:


- *Volatile* memory, baseband generator (BBG) media, where waveform files are played from or edited.
- *Non-volatile* memory, either internal (int) or external (USB) media, where waveform files are stored.

Dual ARB Player

The dual ARB waveform player enables you to play, rename, delete, store, and load (external or internal) waveform files in addition to building waveform sequences. The dual ARB waveform player also provides markers ([page 110](#)), triggering ([page 126](#)), clipping ([page 133](#)), and scaling ([page 142](#)) capabilities.

Most procedures in this section start from the Dual ARB menu, shown below.

Figure 8-1 Dual ARB Softkeys

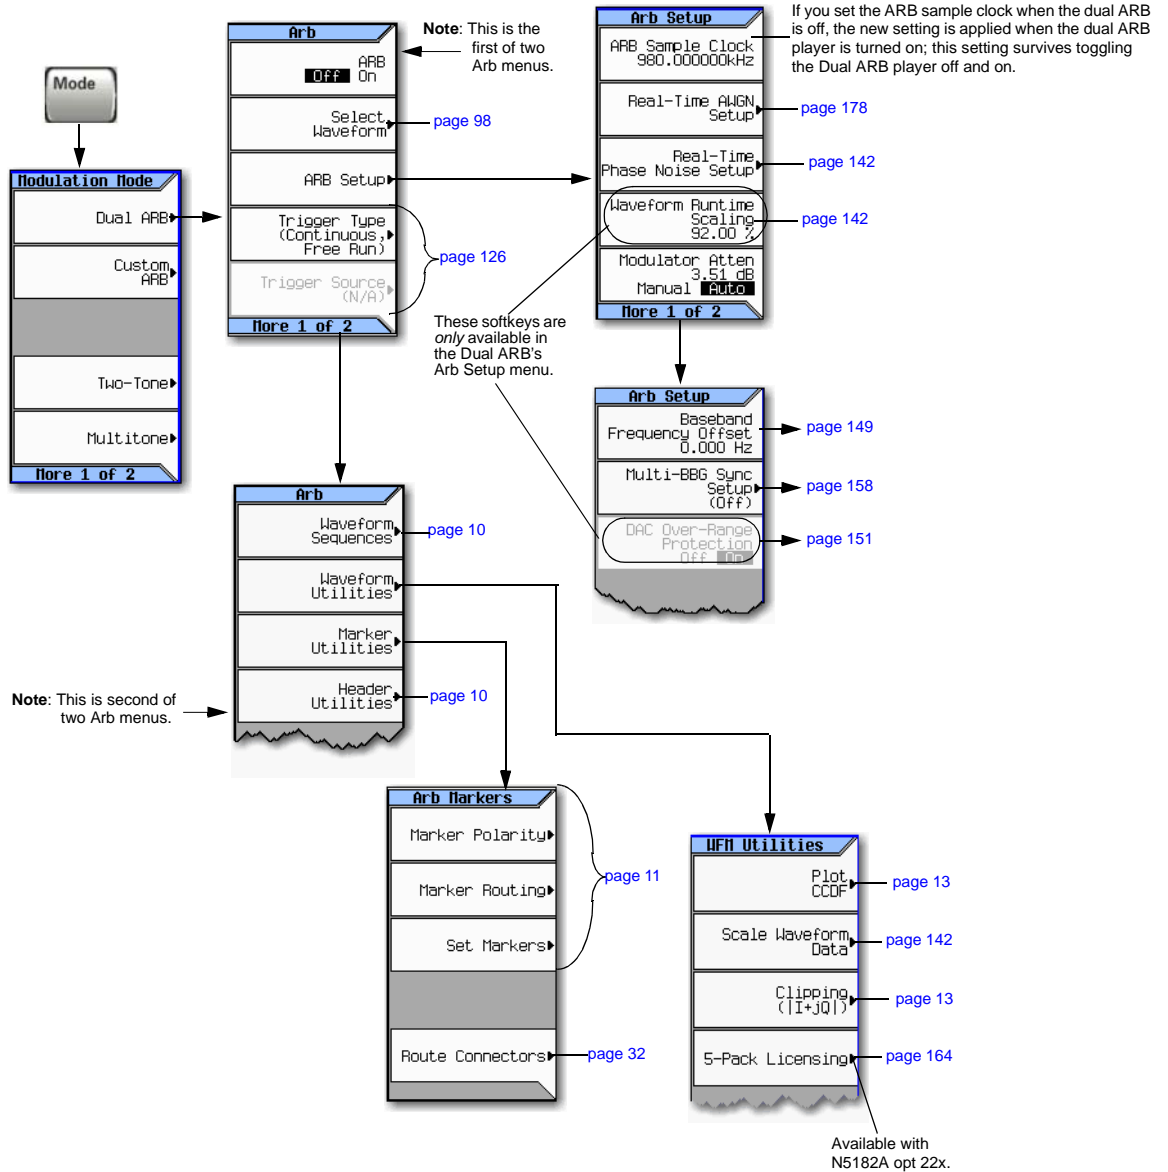

For details on each key, use key help as described on page 26.


Storing, Loading, and Playing a Waveform Segment

Before using this information, you should be familiar with the signal generator’s file menus. If you are not, refer to [Working with Files](#) on page 45 and familiarize yourself with that information.

See also: [Waveform Sequences](#) on page 101.

The signal generator has two types of waveform media: non-volatile (internal or USB), and volatile (BBG). BBG media is also called “working” media, because before you can play, edit, or include a waveform file in a sequence, the waveform file must be loaded into BBG media.

Figure 8-2 Waveform Segment Softkeys

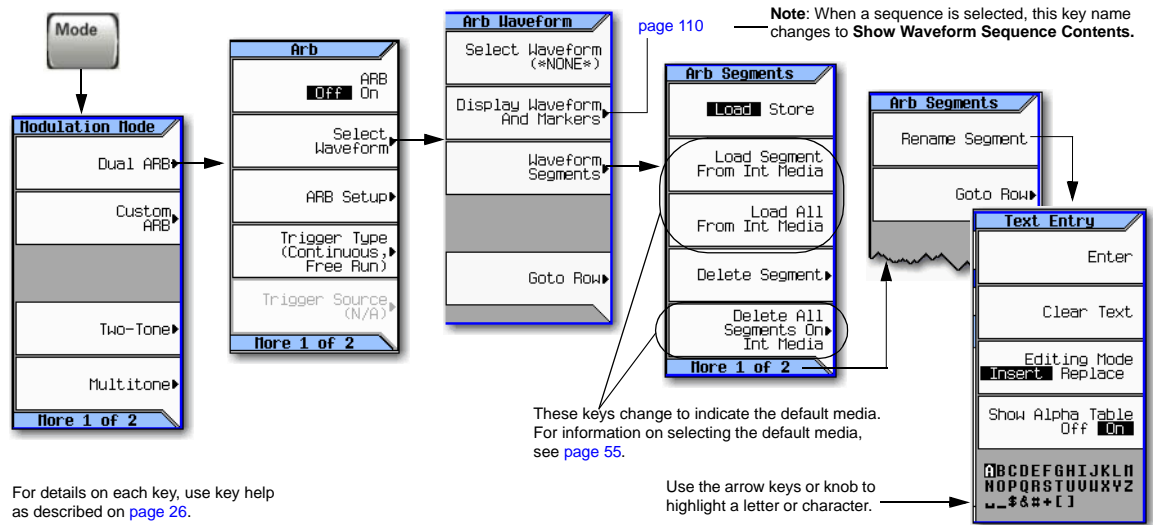

For details on each key, use key help as described on [page 26](#).

Use the arrow keys or knob to highlight a letter or character.

Loading a Waveform Segment into BBG Media

Waveforms must reside in BBG media before they can be played, edited, or included in a sequence. Cycling power or rebooting the signal generator deletes the files in BBG media.

NOTE Each time the instrument powers up, two factory-supplied segments are automatically created in BBG media: `RAMP_TEST_WFM` and `SINE_TEST_WFM`.

There are additional sample waveforms that are available in the internal storage and that can be loaded into memory. Refer to www.agilent.com and search on “Factory Default N5182A” and “waveforms”.

1. Press **Mode** > **Dual ARB** > **Select Waveform** > **Waveform Segments**.
2. Press **Load Store** to highlight **Load**, then, using the arrow keys, highlight the desired waveform segment.
3. If there is already a copy of this segment in the currently selected media and you do not want to overwrite it, rename the waveform segment before you load it (refer to the previous procedure).

4. Press **Load Segment From** *currently selected Media*.

To load *all* files from the currently selected media into BBG media, press **Load All From** *currently selected Media*.

Storing/Renaming a Waveform Segment to Internal or USB Media

Use the following steps to store a copy of a file in BBG memory to the currently selected media (page 55). If you have not downloaded a waveform segment, either refer to the *Programming Guide*, or use one of the factory-supplied segments.

1. Press **Mode > Dual ARB > Select Waveform > Waveform Segments**.
2. Press **Load Store** to highlight Store.
3. Using the arrow keys, highlight the waveform segment you want to store.
4. Optionally, rename the segment.


If there is already a copy of this segment in the currently selected media and you do not want to overwrite it, rename the waveform segment before you store it:

- a. Press **More > Rename Segment > Clear Text**.
 - b. Enter a name for the waveform segment.
 - c. Press **Enter > More**.
 - d. Highlight the waveform segment that was renamed.
5. Press **Store Segment to** *currently selected Media*.
 6. Repeat [Step 3](#) through [Step 5](#) for all segments that you want to store.
- To save *all* segments from BBG media to the currently selected media, press **Store All to** *currently selected Media*.

Playing a Waveform Segment

1. Press **Mode > Dual ARB > Select Waveform**.
2. In the Segment on BBG Media column, highlight the waveform segment you want to play.
3. Press **Select Waveform**.
4. Set **ARB Off On** to On.

This plays the selected waveform segment. Both the I/Q and ARB annunciators turn on, and the waveform modulates the RF carrier.

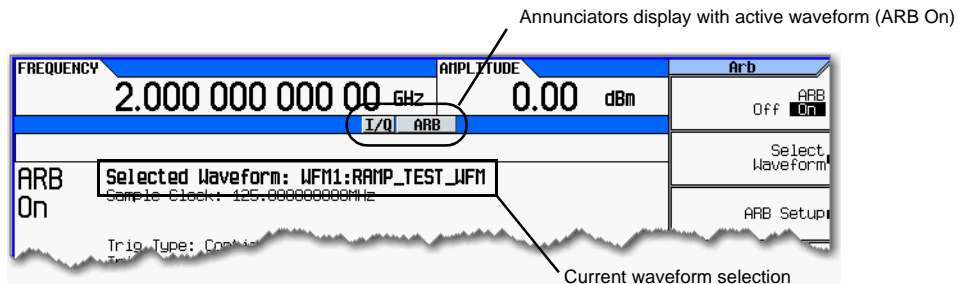


5. Configure the RF Output:

Set the RF carrier frequency and amplitude, and turn on the RF output.

The waveform segment is now available at the signal generator's RF Output connector.

Waveform Sequences

Figure 8-3 Waveform Sequence Softkeys

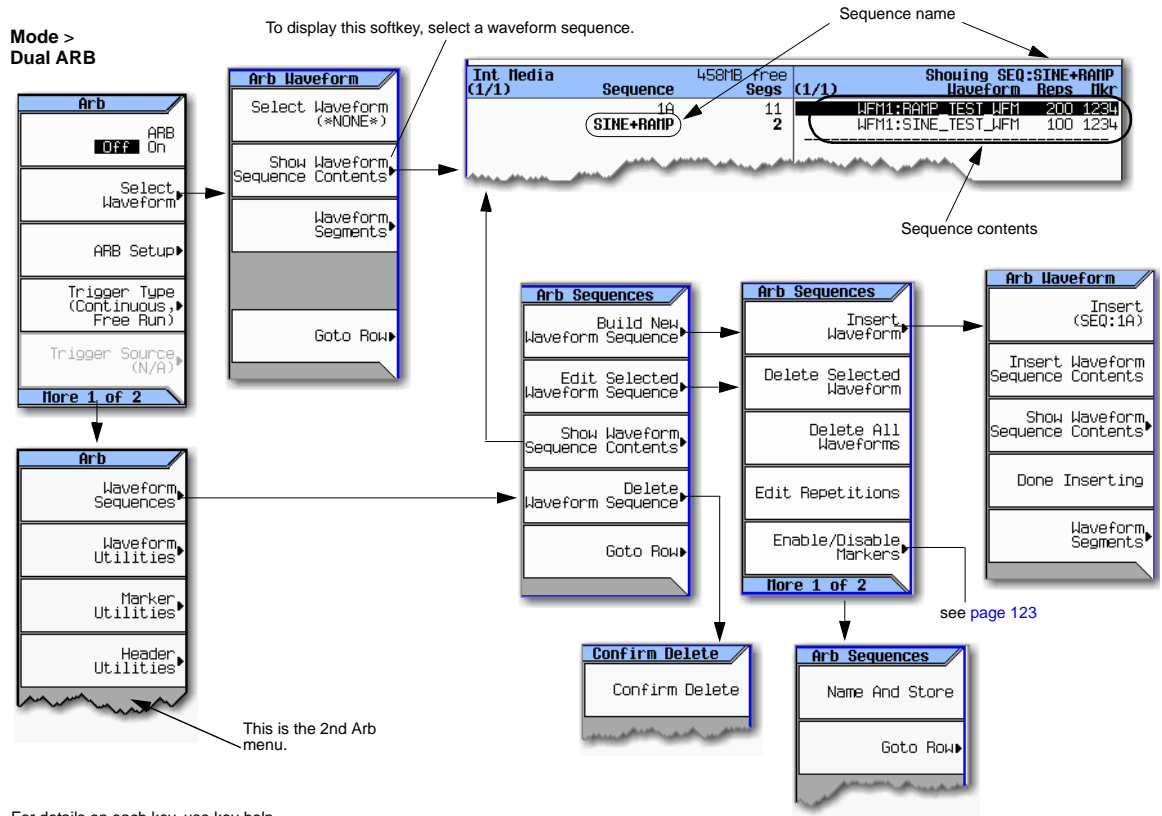


For details on each key, use key help as described on [page 26](#).

A waveform sequence is a file that contains pointers to one or more waveform segments or other waveform sequences, or both. This lets the signal generator play multiple waveform segments, or other sequences, or both thereby eliminating the need to stop waveform playback just to select another waveform.

The segments that a waveform sequence points to are *not* automatically stored when you store the sequence; you must also store the individual segments or they are lost when you turn off or reboot the signal generator. If the segments are located in internal/external media, you must load them into BBG media prior to selecting a waveform sequence (see [page 98](#)). If you attempt to play a sequence without the segments loaded into BBG media, the signal generator reports: ERROR: 629, File format invalid. If this happens and the segments are not stored in internal/external media, you must recreate the segments using the same file names that the sequence points to before you can play the sequence.

Creating a Sequence

A waveform sequence can contain up to 1,024 segments and have both segments and other sequences (nested sequences). The signal generator lets you set the number of times the segments and nested sequences repeat during play back. But there is a difference between repeating a segment versus repeating a nested sequence. Each segment can repeat up to 65,535 times, but no matter how many times a segment repeats, it counts as a single segment. However each repetition of a nested sequence counts as additional segments.

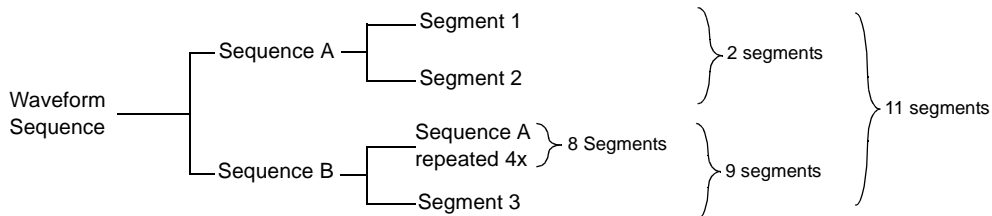

The maximum number of times that a nested sequence can repeat is based on the number of segments in the nested sequence and the remaining number of allowed segments (1,024). For example, with a sequence that contains 24 segments and one nested sequence with 4 segments, the nested sequence is limited to 250 repetitions:

$$24 + (4 \times 250) = 1,024 \text{ maximum number of segments per sequence}$$

Even though there is a limiting factor on the maximum number of times that a nested sequence can repeat, each segment within the nested sequence can repeat up to 65,535 times.

Example

Use the following procedure to create and store a waveform sequence using one repetition each of two different segments.

Assumption: The waveform segments are in BBG media (volatile memory). For information on loading waveform segments into BBG media, see [page 98](#).

1. Select the first segment:
 - a. Press **Mode** > **Dual ARB** > **More** > **Waveform Sequences** > **Build New Waveform Sequence** > **Insert Waveform**.
 - b. Highlight the desired waveform segment and press **Insert**.
2. Select the second segment:
 - a. Highlight the next desired waveform segment and press **Insert**.
 - b. Press **Done Inserting**
3. Name and store the waveform sequence to the Seq file catalog:
 - a. Press **More** > **Name and Store**.
 - b. Enter a file name and press **Enter**.

See also, “[Viewing the Contents of a Sequence](#)” on page 103 and “[Setting Marker Points in a Waveform Segment](#)” on page 117.

Viewing the Contents of a Sequence

There are two ways to view the contents of a waveform sequence:

Through the Waveform Sequences Softkey

1. Press **Mode > Dual ARB > More > Waveform Sequences**.
2. Highlight the desired sequence.
3. Press **Show Waveform Sequence Contents**.

Using the Select Waveform Softkey

1. Press **Mode > Dual ARB > Select Waveform**.
2. In the Sequence On column, highlight the desired waveform sequence.
3. Press **Show Waveform Sequence Contents**.

Editing a Sequence

When editing a waveform sequence, you can:

- change the number of times each segment or nested sequence plays
- delete segments or nested sequences from the sequence
- add segments or nested sequences to the sequence
- toggle markers on and off (described on [page 123](#))
- save changes either to the current waveform sequence or as a new sequence

If you exit the sequence editing menu before saving changes, the changes are lost.

Sequences save to the Seq file catalog.

CAUTION If you edit and resave a segment used in a sequence, the sequence does not automatically update the RMS value in its header. You must select and update the sequence header information ([page 105](#)).

Use the following steps to edit a sequence that has two different segments so that the first segment repeats 100 times and the second segment repeats 200 times, then save the changes.

Assumption: A waveform sequence that has two different segments has been created and stored (see previous example on [page 102](#)).

1. Select the sequence:
Press **Mode > Dual ARB > More > Waveform Sequences > highlight the desired sequence > Edit Selected Waveform Sequence**.
2. Change the first segment so that it repeats 100 times:
Highlight the first segment entry and press **Edit Repetitions > 100 > Enter**.
The cursor moves to the next entry.
3. Change the repetition for the selected entry to 200:
Press **Edit Repetitions > 200 > Enter**.
4. Save the changes made in the previous steps:
Press **More > Name and Store > Enter**.

To save the changes as a *new* sequence:

- a. Press **More > Name and Store > Clear Text**.
- b. Enter a file name (for example, SINE100+RMP200).
- c. Press **Enter**.

The edited sequence saves as a new waveform sequence.


Playing a Sequence

If you have not created a waveform sequence, refer to “Creating a Sequence” on page 102.

NOTE To play a waveform segment individually or as part of a waveform sequence, the segment must reside in BBG media. See also, “Loading a Waveform Segment into BBG Media” on page 98.

1. Select a waveform sequence:
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. Highlight a waveform sequence (for this example, SINE100+RMP200) from the Sequence On column.
 - c. Press **Select Waveform**.

The display shows the currently selected waveform (for example, Selected Waveform: SEQ:SINE100+RMP200).

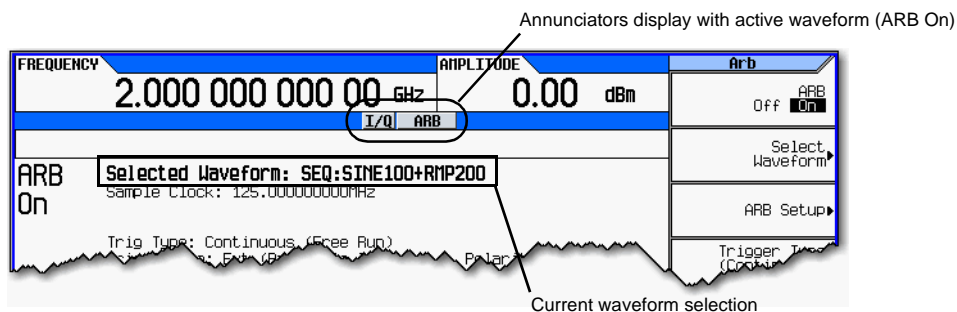

2. Generate the waveform:

Press **ARB Off On** to On.


This plays the selected waveform sequence. During the waveform sequence generation, both the I/Q and ARB annunciators turn on, and the waveform modulates the RF carrier.
3. Configure the RF output:
 - a. Set the RF carrier frequency.
 - b. Set the RF output amplitude.
 - c. Turn on the RF output.

The waveform sequence is now available at the signal generator's RF OUTPUT connector.

Saving a Waveform's Settings & Parameters

This section describes how to edit and save a file header. When you download only a waveform file (I/Q data, which the signal generator treats as a waveform segment), the signal generator automatically generates a file header and a marker file with the same name as the waveform file. Initially the file header has no signal generator settings saved to it, and the marker file consists of all zeros. For a given waveform, you can save signal generator settings and parameters in its file header and marker settings in its marker file (page 110); when you load a stored waveform file into BBG media, the file header and marker file settings automatically apply to the signal generator so that the dual ARB player sets up the same way each time the waveform file plays.

Figure 8-4 Header Utilities Softkeys

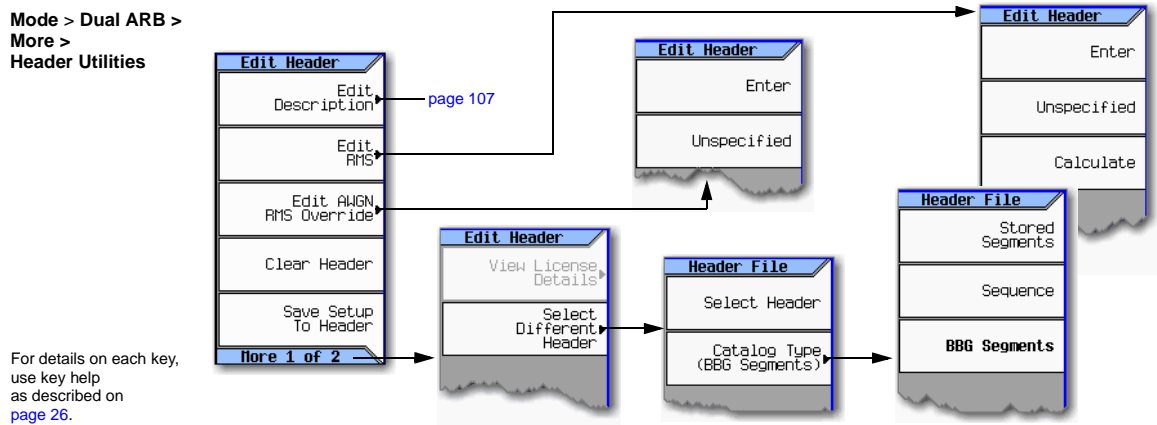

When you create a waveform sequence (as described on page 102), the signal generator automatically creates a waveform sequence header that takes priority over the individual waveform segment headers. During a waveform sequence playback, the segment headers are ignored, except to verify that all required options are installed. Storing a waveform sequence also stores its file header.

Some of the current signal generator settings shown in the file header appear as part of the softkey labels, and others appear in the dual ARB summary display, shown in the following example.

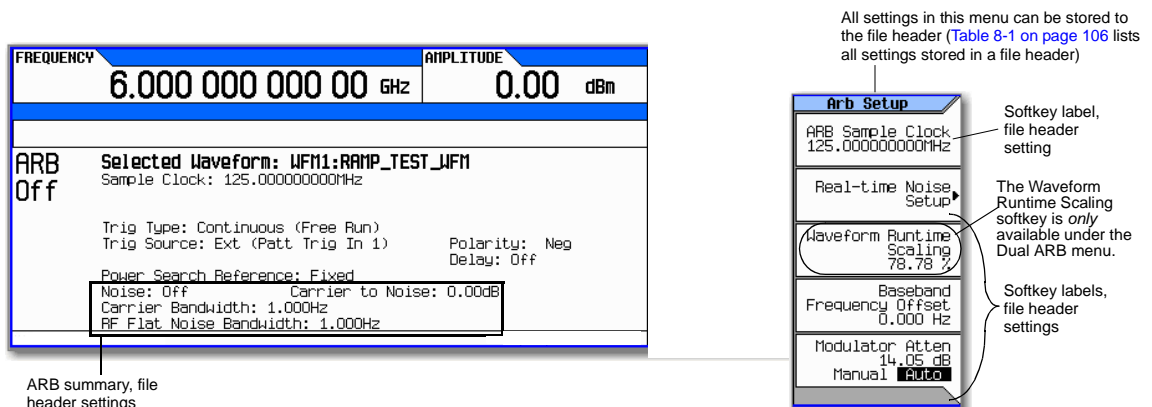


Table 8-1 File Header Entries

32-Character Description	A description entered for the header, such as a the waveform's function (saved/edited with the Edit Description softkey, see Figure 8-4).
Sample Rate	The waveform playback rate. This is the ARB sample clock rate, set in the Arb Setup menu (shown in Figure 8-1 on page 97).
Runtime Scaling	The Runtime scaling value is applied in real-time while the waveform is playing. This setting can be changed only for files playing in the dual ARB player (see page 146).
RMS	When the modulator attenuation setting (see page 97) is set to Auto, this value is used to calculate the I/Q modulator attenuation setting to optimize ACPR. Value: 0 to 1.414213562
Marker 1...4 Polarity	Marker polarity can be positive or negative (described on page 122).
ALC Hold Routing	Which marker, if any, implements the ALC hold function (described on page 112), which holds the ALC at its current level when the marker signal is low. All waveforms generated in the signal generator have a marker on the first sample point. To see the results from the three routing selections, you may need to select a range of sample (marker) points (see "Setting Marker Points in a Waveform Segment" on page 117).
RF Blank Routing	Which marker, if any, implements the RF blanking function (described on page 120) when the marker signal is low. RF blanking also uses ALC hold. There is no need to select the ALC Hold Routing for the same marker when you are using the RF Blank Routing function. When the marker signal goes high, RF blanking discontinues.
Mod Attenuation	The I/Q modulator attenuation setting (set in the Arb Setup menu shown in Figure 8-1 on page 97).
BB Freq Offset	The baseband frequency offset, in Hz (see page 149).
AWGN: State	Indicated whether real-time noise is on (1) or off (0) (see page 177).
AWGN: C/N Ratio	Carrier to noise ration, in dB (see page 180).
AWGN: Carrier BW	Bandwidth over which the noise power is integrated, in Hz (see page 180).
AWGN: Noise BW	Bandwidth of the noise, in Hz (see page 180).
AWGN: Carrier RMS	The carrier RMS across the carrier bandwidth (see page 180).
Phase Noise State	Indicated whether phase noise is on (1) or off (0) (see page 184).
Phase Noise F1	The start frequency for the level mid-frequency characteristics (see page 184).
Phase Noise F2	The end frequency for the level mid-frequency characteristics (see page 184).
Phase Noise Lmid	The amplitude for the level mid-frequency characteristics (see page 184).
Over-Range Protect	Indicated whether DAC Over-Range Protection is on (1) or off (0) (see page 188).
Unique Waveform Id	0 = no Id; once an Id is assigned, it cannot be changed.
License Required	Indicates whether a license is required to play the waveform. See also: "Viewing Options and Licenses" on page 24
Can be Read Out	Indicates whether the waveform can be queried through SCPI or FTP.

Viewing and Modifying Header Information

The following example uses the factory-supplied waveform file RAMP_TEST_WFM.

1. From BBG media, select the waveform RAMP_TEST_WFM:
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. In the Segment On column, highlight the waveform RAMP_TEST_WFM.
 - c. Press **Select Waveform**.

2. Open the Header Utilities menu:

Press **More > Header Utilities**

The **Figure 8-5** shows the default file header for the factory-supplied waveform RAMP_TEST_WFM. The Header Field column lists the file header parameters; use the **Page Down** key to see them all.

The Saved Header Settings column shows that most of the settings are Unspecified. Unspecified means that there is no setting saved for that particular parameter.

The Current Inst. Settings column shows the current signal generator settings. In this example, these are the settings that you will save to the file header.

NOTE If a setting is unspecified in the file header, the signal generator uses its current value for that setting when you select and play the waveform.

Figure 8-5 Example File Header

Mode > Dual ARB > More > Header Utilities

The screenshot shows the following interface elements:

- FREQUENCY:** 6.000 000 000 00 GHz
- AMPLITUDE:** -144.00 dBm
- Edit Header:** Edit Description, Edit RMS, Edit AWGN RMS Override, Clear Header, Save Setup To Header
- File Header Information:** RAMP_TEST_WFM
- Header Field:** Saved Header Settings, Current Inst. Settings
- Description:**

Header Field	Saved Header Settings	Current Inst. Settings
Sample Rate	Unspecified	125.000000000Hz
Runtime Scaling	78.78 %	78.78 %
RMS	0.814852207	N/A
Marker 1 Polarity	Unspecified	Pos
Marker 2 Polarity	Unspecified	Pos
Marker 3 Polarity	Unspecified	Pos
Marker 4 Polarity	Unspecified	Pos
ALC Hold Routing	Unspecified	None

Annotations:

- The name of the waveform file.
- The description can be up to 32-characters.
- Opens a menu for manually defining the carrier RMS value to use for calculating the AWGN: Carrier RMS value in the Header Field.
- Resets the saved header settings entries to default settings
- Default header settings
- Current signal generator settings
- To calculate the RMS waveform voltage: Press **Calculate**
- Then refer to Header Field information.
- Note: For greater accuracy, if the waveform has long rise/fall times, a DC offset, or noise* already added to the waveform (for a bursted signal), it is recommended that the Edit RMS and Edit AWGN RMS Override softkeys are used for the best measurement accuracy.
- *Option 403 Real-time AWGN does not affect the Header Field RMS value. But, noise added to the waveform prior to downloading and playing in the signal generator does affect the Header Field RMS value.

3. Save the information in the Current Inst. Settings column to the file header:

Press **Save Setup To Header**.

Both the Saved Header Settings column and the Current Inst. Settings column now display the same values; the Saved Header Settings column lists the settings saved in the file header.


4. Edit and Update Settings

a. Return to the ARB Setup menu:
 Press **Return > More > ARB Setup**.

From this menu you can access some of the signal generator settings that are saved to the file header. [Figure 8-1 on page 97](#) shows the ARB Setup softkeys used in the following steps.

- b. Set the ARB sample clock to 5 MHz:
 Press **ARB Sample Clock > 5 > MHz**.
- c. Set waveform runtime scaling to 60%:
 Press **Waveform Runtime Scaling > 60 > %**.
- d. Return to the Header Utilities menu:
 Press **Return > More > Header Utilities**.

As shown in the following figure, the Current Inst. Settings column now reflects the changes to the current signal generator setup, but the *saved* header values have not changed.

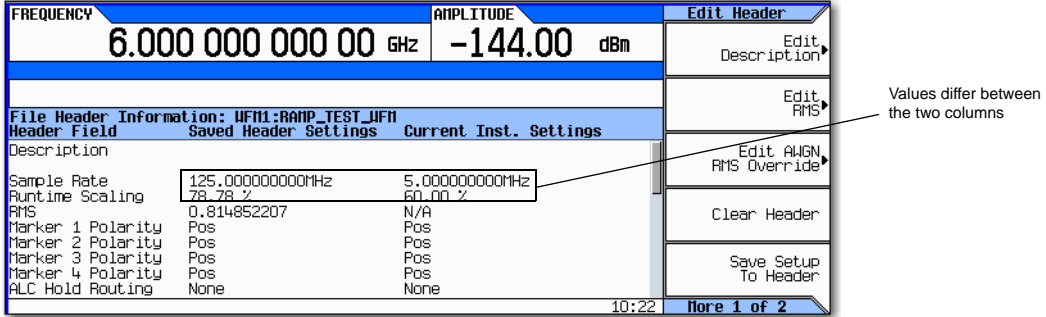

e. Save the current settings to the file header:
 Press the **Save Setup To Header** softkey.

The settings from the Current Inst. Settings column now appear in the Saved Header Settings column. This saves the new current instrument settings to the file header.

If you change any of the signal generator settings listed in the file header after you select the waveform file, the changed setting(s) appear in the file header's Current Inst. Settings column and are used instead of the saved header settings. To reapply the saved header settings, reselect the waveform for playback.

Viewing & Editing a Header without Selecting the Waveform

As described on [page 107](#), you can view and edit a waveform's header information after you select the waveform; you can also edit waveform header information without selecting a waveform, or for another waveform than the one that is currently selected.

1. Access the file header utilities menu:

Press **Mode** > **Dual ARB** > **More** > **Header Utilities** > **More** > **Select Different Header**.

The signal generator displays an alphabetical list of the waveform files in the media that was last selected. The following figure shows an example of the factory-supplied waveforms in BBG media.

Active catalog

Active media

Active waveform catalog

Files in BBG media

Header File

Select Header

Catalog Type (BBG Segments)

Header File

Stored Segments

Sequence

BBG Segments

Catalogs that enable you to view files in the active media. For details on selecting the active media, see [page 47](#).

Type:
WFM1 = Volatile Segment
NVWFM = Non-Volatile Segment
SEQ = Sequence

For details on each key, use key help as described on [page 26](#).

File Name	Type	Size	Modified
1 RAMP_TEST_WFM	WFM1	800	--/--/-- :--
2 SINE_TEST_WFM	WFM1	800	--/--/-- :--

2. If the desired catalog is not displayed, select it.
3. Highlight the desired waveform file and press **Select Header**.

The signal generator displays the file header for the selected waveform file.

4. To edit the header, press **More**, and proceed as described in [Step 4 on page 108](#) ([Viewing and Modifying Header Information](#) section).

Using Waveform Markers

The signal generator provides four waveform markers to mark specific points on a waveform *segment*. When the signal generator encounters an enabled marker, an auxiliary signal is routed to a rear panel event output that corresponds to the marker number.

- Event 1 is available at both the EVENT 1 BNC connector (see [page 14](#)), and a pin on the AUXILIARY I/O connector (see [page 15](#)).
- Event 2 is available at both the TRIG OUT BNC connector (see [page 12](#)), and a pin on the AUXILIARY I/O connector (see [page 15](#)).
- Events 3 and 4 are available at pins on the AUXILIARY I/O connector (see [page 15](#)).

You can use an auxiliary output signal to synchronize another instrument with the waveform, or as a trigger signal to start a measurement at a given point on a waveform.

You can also configure markers to initiate ALC hold or RF Blanking (which includes ALC hold). Refer to [“Using Waveform Markers” on page 110](#) for details.

When you download a waveform file that does not have a marker file associated with it, the signal generator creates a marker file without any marker points. Factory-supplied segments (RAMP_TEST_WFM and SINE_TEST_WFM) have a marker point on the first sample for all four markers.

The following procedures demonstrate how to use markers while working in the dual ARB player. These procedures also discuss two types of points: a *marker point* and a *sample point*. A marker point is a point at which a given marker is set on a waveform; you can set one or more marker points for each marker. A *sample point* is one of the many points that compose a waveform.

There are three basic steps to using waveform markers:

[“Clearing Marker Points from a Waveform Segment” on page 116](#)

[“Setting Marker Points in a Waveform Segment” on page 117](#)


[“Controlling Markers in a Waveform Sequence” on page 123](#)

This section also provides the following information:

- [“Waveform Marker Concepts” on page 111](#)
- [“Accessing Marker Utilities” on page 115](#)
- [“Viewing Waveform Segment Markers” on page 116](#)
- [“Viewing a Marker Pulse” on page 119](#)
- [“Using the RF Blanking Marker Function” on page 120](#)
- [“Setting Marker Polarity” on page 122](#)

Waveform Marker Concepts

The signal generator's Dual ARB provides four waveform markers for use on a waveform segment. You can set each marker's polarity and marker points (on a single sample point or over a range of sample points). Each marker can also perform ALC hold, or RF Blanking and ALC hold.

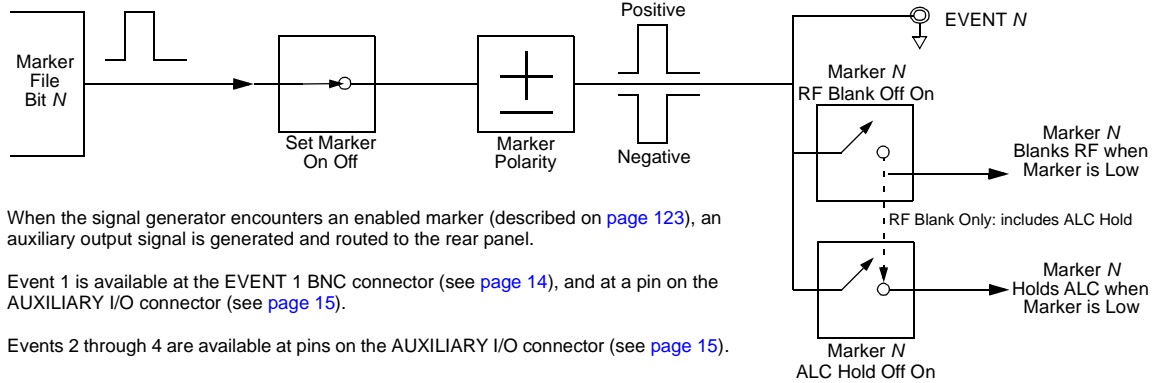

When the signal generator encounters an enabled marker (described on [page 123](#)), an auxiliary output signal is generated and routed to the rear panel.

Event 1 is available at the EVENT 1 BNC connector (see [page 14](#)), and at a pin on the AUXILIARY I/O connector (see [page 15](#)).

Events 2 through 4 are available at pins on the AUXILIARY I/O connector (see [page 15](#)).

Marker Signal Response

The signal generator aligns the marker signals with the I and Q signals at the baseband generator. However some settings such as amplitude, filters, and so forth within the RF output path can create delays between the marker EVENT output signal and the modulated RF output. When using the marker EVENT output signal, observe the signals (marker relative to modulated RF) for any latency, and if needed, reset the marker point positions, include delay ([page 155](#)), or both.

Marker File Generation

Downloading a waveform file (as described in the *Programming Guide*) that does not have a marker file associated with it causes the signal generator to automatically create a marker file, but does *not* place any marker points.

Marker Point Edit Requirements

Before you can modify a waveform segment's marker points, the segment must reside in BBG media (see "Loading a Waveform Segment into BBG Media" on [page 98](#)).

Saving Marker Polarity and Routing Settings

Marker polarity and routing settings remain until you reconfigure them, preset the signal generator, or cycle power. To ensure that a waveform uses the correct settings when it is played, set the marker polarities or routing (RF Blanking and ALC Hold) and save the information to the file header ([page 105](#)).

NOTE When you use a waveform that does not have marker routings and polarity settings stored in the file header, and the previously played waveform used RF Blanking, ensure that you set RF Blanking to **None**. Failure to do so can result in no RF output or a distorted waveform.

ALC Hold Marker Function


While you can set a marker function (described as **Marker Routing** on the softkey label) either before or after you set marker points (page 117), setting a marker function before setting marker points may cause power spikes or loss of power at the RF output.

Use the ALC hold function by itself when you have a waveform signal that incorporates idle periods, burst ramps, or when the increased dynamic range encountered with RF blanking (page 120) is not desired.

The ALC hold marker function holds the ALC circuitry at the *average* value of the sampled points set by the marker(s). For both positive and negative marker polarity, the ALC samples the RF output signal (the carrier plus any modulating signal) when the marker signal goes high:

- Positive: The signal is sampled during the on marker points.
- Negative: The signal is sampled during the off marker points.

NOTE Because it can affect the waveform's output amplitude, do not use the ALC hold for longer than 100 ms. For longer time intervals, refer to "Power Search Mode" on page 74.


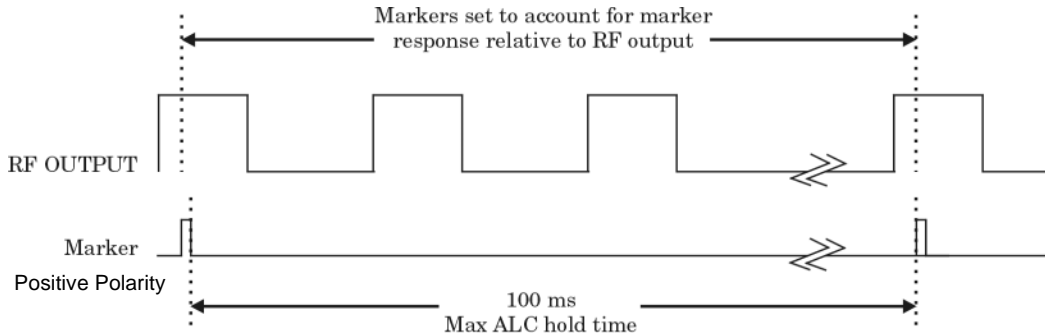


CAUTION Incorrect ALC sampling can create a sudden unlevelled condition that may create a spike in the RF output, potentially damaging a DUT or connected instrument. To prevent this condition, ensure that you set markers to let the ALC sample over an amplitude that accounts for the higher power levels encountered within the signal.

Example of Correct Use

Waveform: 1022 points
Marker range: 95-97
Marker polarity: Positive


This example shows a marker set to sample the waveform's area of highest amplitude. Note that the marker is set well before the waveform's area of lowest amplitude. This takes into account any response difference between the marker and the waveform signal.

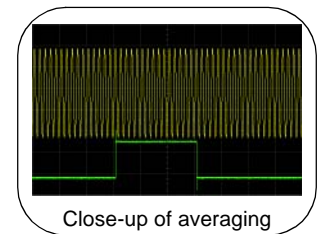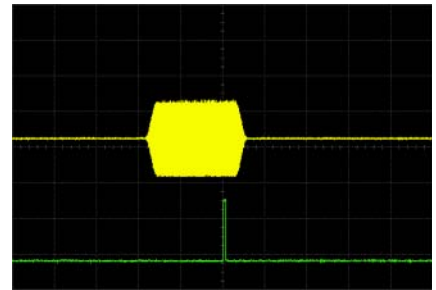

Close-up of averaging

The ALC samples the waveform when the marker signal goes high, and uses the average of the sampled waveform to set the ALC circuitry.


Here the ALC samples during the *on* marker points (positive polarity).

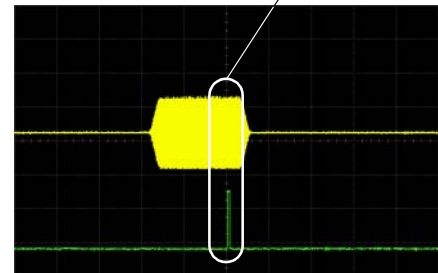

Example of Incorrect Use

Waveform: 1022 points
Marker range: 110-1022
Marker polarity: Positive


This example shows a marker set to sample the low part of the same waveform, which sets the ALC modulator circuitry for that level; this usually results in an unlevelled condition for the signal generator when it encounters the high amplitude of the pulse.

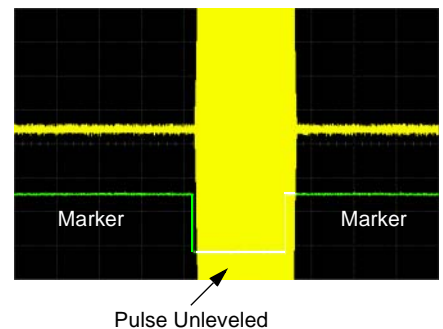

Example of Incorrect Use


Waveform: 1022 points
Marker range: 110-1022
Marker polarity: Negative

This figure shows that a negative polarity marker goes low during the marker *on* points; the marker signal goes high during the *off* points. The ALC samples the waveform during the *off* marker points.

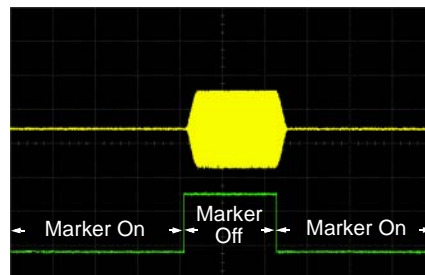

Sample range begins on first point of signal

Sampling both on and off time sets the modulator circuitry incorrectly for higher signal levels. Note the increased amplitude at the beginning of the pulse.


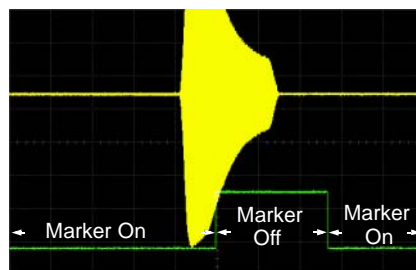


Negative range set between signal and off time

Accessing Marker Utilities

Mode > Dual ARB > More > Marker Utilities

For details on each key, use key help as described on [page 26](#).

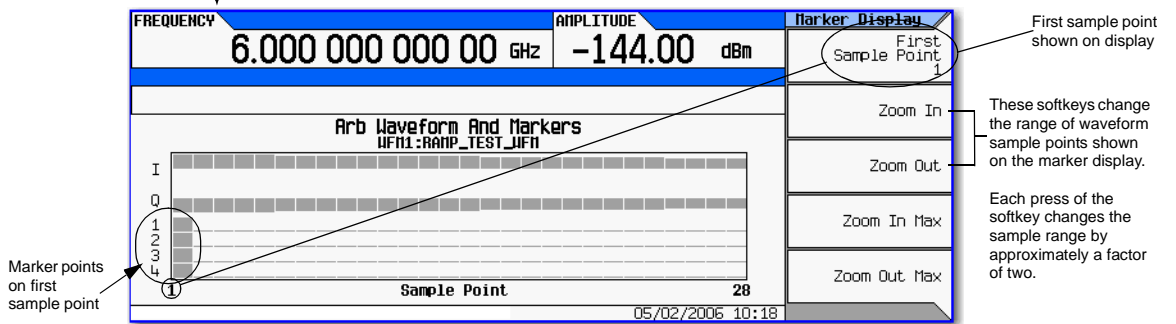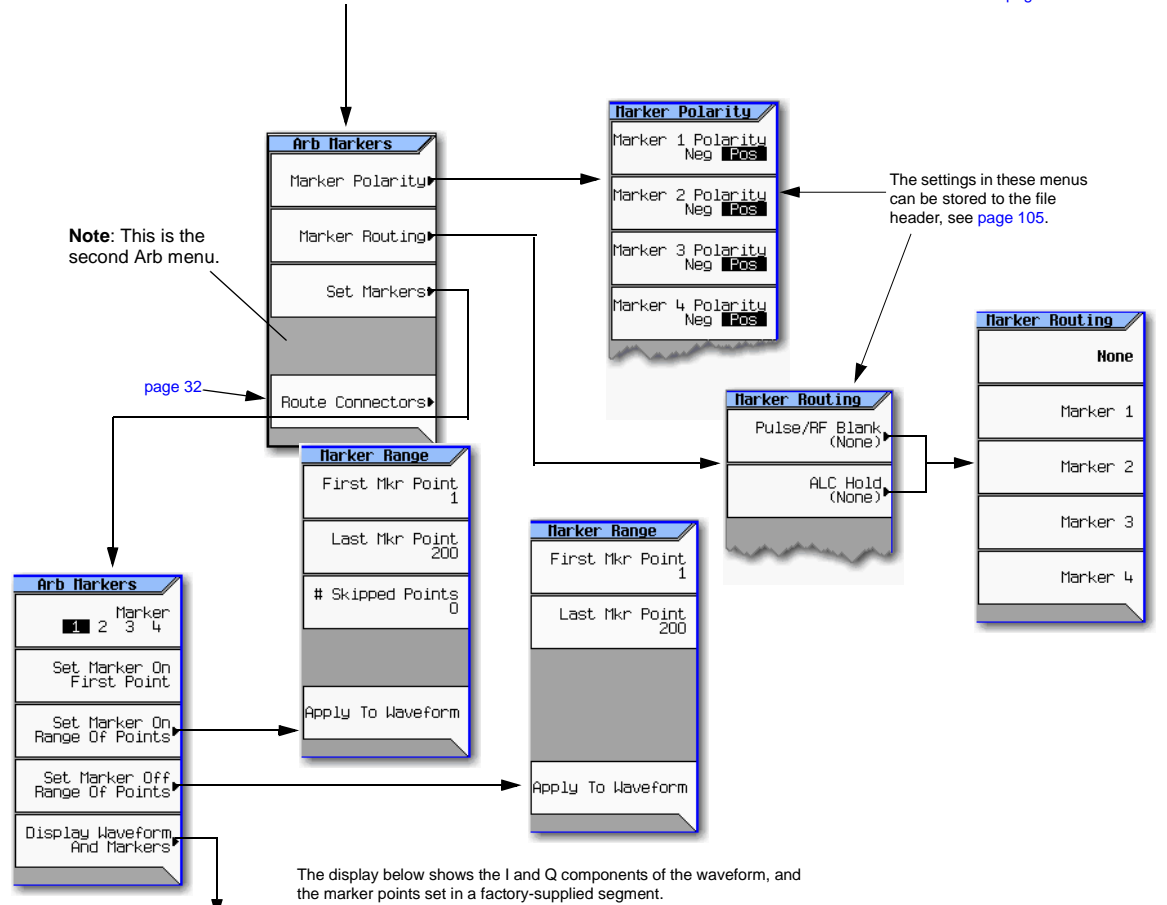

Viewing Waveform Segment Markers

Markers are applied to waveform segments. Use the following steps to view the markers set for a segment (this example uses the factory-supplied segment, SINE_TEST_WFM).

1. In the second Arb menu (page 115), press **Marker Utilities > Set Markers**.
2. Highlight the desired waveform segment (in this example, SINE_TEST_WFM).
3. Press **Display Waveform and Markers > Zoom in Max**.
The maximum zoom in range is 28 points.

Experiment with the Zoom functions to see how they display the markers.

The display can show a maximum of 460 points; displayed waveforms with a sample point range greater than 460 points may not show the marker locations.

Clearing Marker Points from a Waveform Segment

When you set marker points they do not replace points that already exist, but are set *in addition* to existing points. Because markers are cumulative, before you set points, view the segment (page 116) and remove any unwanted points. With all markers cleared, the level of the event output signal is 0V. To clear marker points on a segment, the segment must reside in BBG media (page 98).

Clearing All Marker Points

1. In the second Arb menu (page 115), press **Marker Utilities > Set Markers**.
2. Highlight the desired waveform segment (in this example, SINE_TEST_WFM).
3. Highlight the desired marker number: Press **Marker 1 2 3 4**.
4. For the selected marker number, remove all marker points in the selected segment:
 - a. Press **Set Marker Off Range of Points**.

Notice that the softkeys for the first and last marker points correspond with the length of the waveform. The factory-supplied waveform (SINE_TEST_WFM) contains 200 samples. To clear all set marker points, the range must equal to the length of the waveform.

- b. Press **Apply To Waveform > Return**.
5. Repeat from Step 3 for any remaining marker points that you want to remove from the other markers.

Clearing a Range of Marker Points


The following example uses a waveform with marker points (Marker 1) set across points 10–20. This makes it easy to see the affected marker points. The same process applies whether the existing points are set over a range or as a single point (page 117).⁴

1. In the second Arb menu (page 115), press **Marker Utilities > Set Markers**, then select Marker 1.
2. Set the first sample point that you want off (for this example, 13):
Press **Set Marker Off Range Of Points > First Mkr Point > 13 > Enter**.
3. Set the last marker point in the range that you want off to a value less than or equal to the number of points in the waveform, *and* greater than or equal to the value set in Step 2 (for this example, 17):

Press **Last Mkr Point > 17 > Enter > Apply To Waveform > Return.**

This turns off all marker points for the active marker within the range set in [Steps 2 and 3](#), as shown at right.

How to view markers is described on [page 116](#).

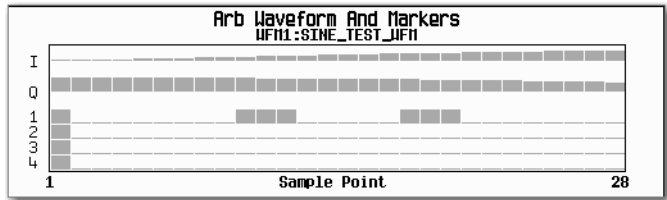

Clearing a Single Marker Point

Use the steps described in [“Clearing a Range of Marker Points”](#) on [page 116](#), but set both the first and last marker point to the value of the point you want to clear. For example, if you want to clear a marker on point 5, set both the first and last value to 5.

Setting Marker Points in a Waveform Segment

To set marker points on a segment, the segment must reside in BBG media ([page 98](#)).

When you set marker points, they do not replace points that already exist, but are set *in addition* to existing points. Because markers are cumulative, before you set marker points within a segment, view the segment ([page 116](#)) and remove any unwanted points ([page 116](#)).

Placing a Marker Across a Range of Points

1. In the second Arb menu ([page 115](#)), press **Marker Utilities > Set Markers.**

2. Highlight the desired waveform segment.

3. Select the desired marker number: Press **Marker 1 2 3 4**

4. Set the first sample point in the range (in this example, 10):


Press **Set Marker On Range Of Points > First Mkr Point > 10 > Enter.**

5. Set the last marker point in the range to a value less than or equal to the number of points in the waveform, *and* greater than or equal to the first marker point (in this example, 20):

Press **Last Mkr Point > 20 > Enter.**

6. Press **Apply To Waveform > Return.**

This sets a range of waveform marker points. The marker signal starts on sample point 10, and ends on sample point 20, as shown in the following figure.

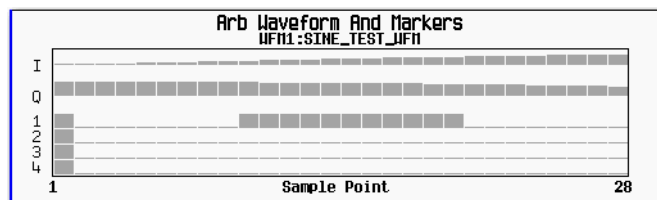

How to view markers is described on

Placing a Marker on a Single Point

On the First Point

1. In the second Arb menu ([page 115](#)), press **Marker Utilities > Set Markers**.
2. Highlight the desired waveform segment.
3. Select the desired marker number:
Press **Marker 1 2 3 4**.
4. Press **Set Marker On First Point**.

This sets a marker on the first point in the segment for the marker number selected in [Step 3](#).

On Any Point

Use the steps described in [“Placing a Marker Across a Range of Points”](#) on [page 117](#), but set both the first and last marker point to the value of the point you want to set. For example, if you want to set a marker on point 5, set both the first and last value to 5.

Placing Repetitively Spaced Markers


The following example sets markers across a range of points and specifies the spacing (skipped points) between each marker. You must set the spacing *before* you apply the marker settings; you cannot apply skipped points to a previously set range of points.

1. Remove any existing marker points ([page 111](#)).
2. In the second Arb menu ([page 115](#)), press **Marker Utilities > Set Markers**.
3. Highlight the desired waveform segment.
4. Select the desired marker number:
Press **Marker 1 2 3 4**.
5. Set the first sample point in the range (in this example, 5):
Press **Set Marker On Range Of Points > First Mkr Point > 5 > Enter**.
6. Set the last marker point in the range. (The last marker point value must always be less than or equal to the number of points in the waveform, *and* greater than or equal to the first marker point, in this example, 25):
Press **Last Mkr Point > 25 > Enter**.
7. Enter the number of sample points that you want skipped (in this example, 1):
Press **# Skipped Points > 1 > Enter**.
8. Press **Apply To Waveform > Return**.

This causes the marker to occur on every other point (one sample point is skipped) within the marker point range, as shown at right.

How to view markers is described on [page 116](#).


One application of the skipped point feature is the creation of a clock signal as the EVENT output.

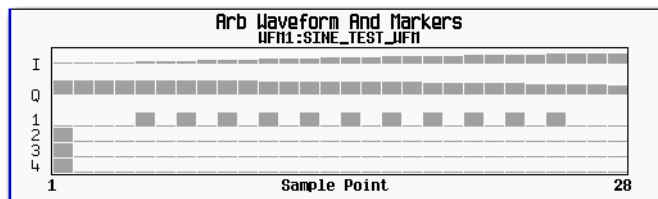

Viewing a Marker Pulse

When a waveform plays (page 104), you can detect a set and enabled marker's pulse at the rear panel event connector/Aux I/O pin that corresponds to that marker number. This example demonstrates how to view a marker pulse generated by a waveform segment that has at least one marker point set (page 117). The process is the same for a waveform sequence.


This example uses the factory-supplied segment, SINE_TEST_WFM in the dual ARB Player. Factory-supplied segments have a marker point on the first sample point for all four markers, as shown.

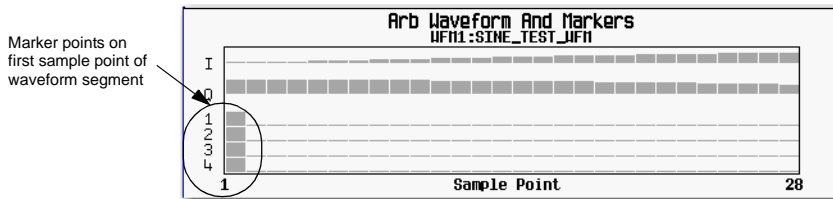

How to view markers is described on page 116

1. In the first Arb menu (page 97), press **Select Waveform**.
2. Highlight the SINE_TEST_WFM segment and press **Select Waveform**.
3. Press **ARB Off On** to On.
4. Connect the Agilent MXG's rear-panel Q OUT output to the oscilloscope's channel 1 input.
5. Connect the signal generator's rear-panel EVENT 1 output to the oscilloscope's channel 2 input.

When marker 1 is present, the Agilent MXG outputs a signal through EVENT 1 as shown in the following example.


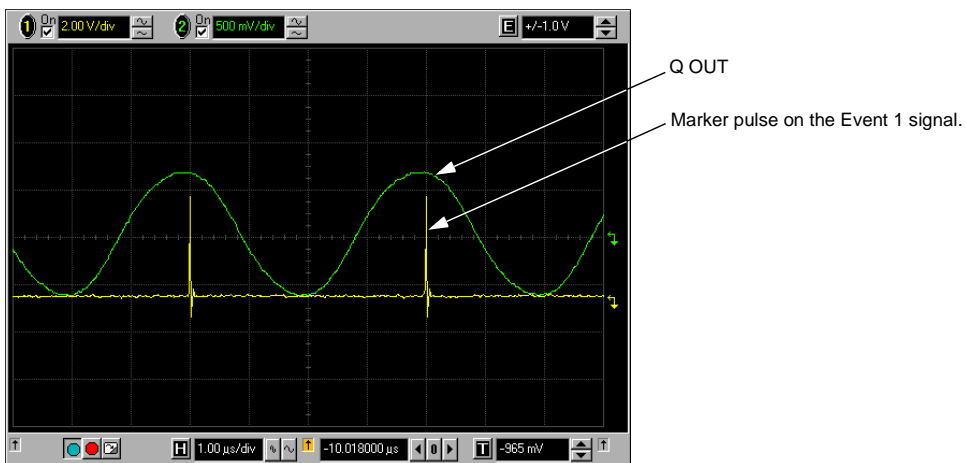


Using the RF Blanking Marker Function

While you can set a marker function (described as **Marker Routing** on the softkey label in the Marker Utilities menu) either before or after setting the marker points ([page 117](#)), setting a marker function before you set marker points may change the RF output. RF Blanking includes ALC hold (described on [page 112](#), note **Caution** regarding unlevelled power). The signal generator blanks the RF output when the marker signal goes low. This example is a continuation of the previous example, [Viewing a Marker Pulse](#).

1. Using the factory-supplied segment SINE_TEST_WFM, set Marker 1 across points 1–180 ([page 117](#)).
2. From the **Marker Routing** softkey menu, assign RF Blanking to Marker 1:
In the second Arb menu ([page 115](#)), press **Marker Utilities** > **Marker Routing** > **Pulse/RF Blank** > **Marker**

1.

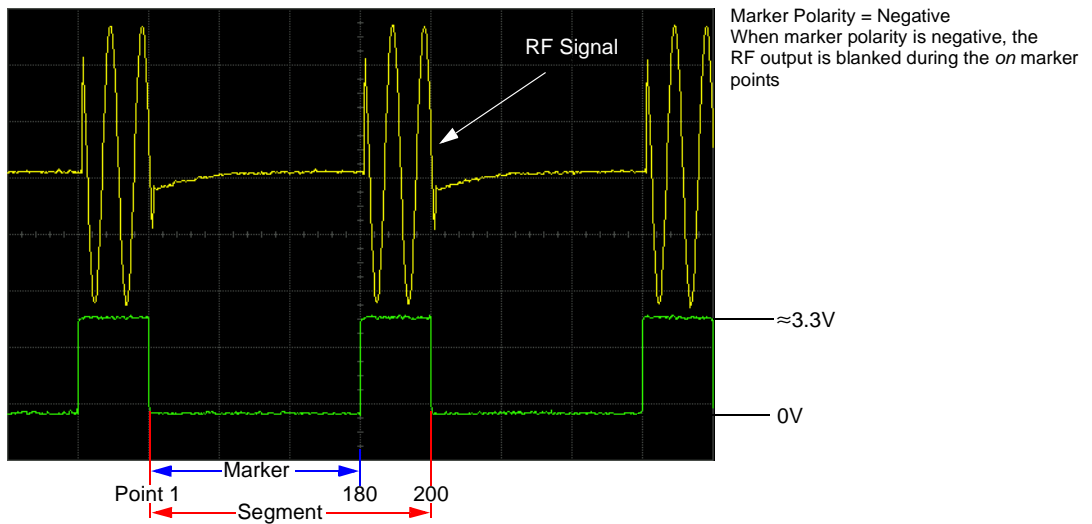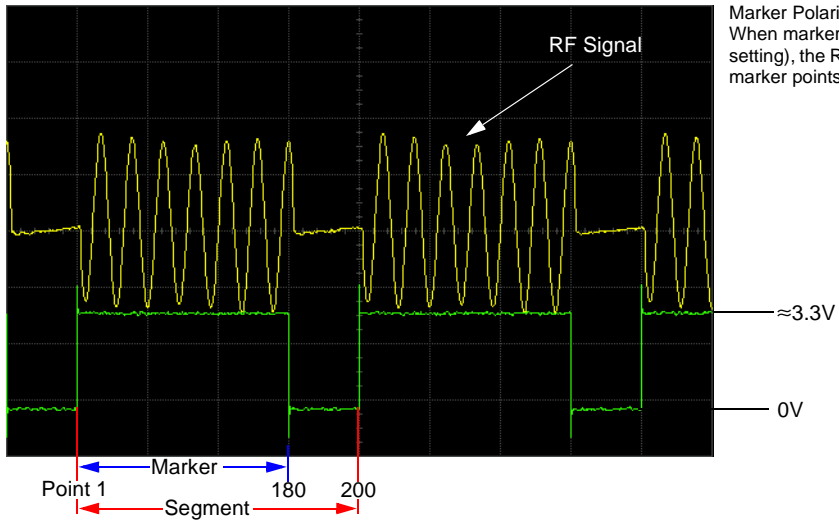

Setting Marker Polarity

Setting a negative marker polarity inverts the marker signal.

1. In second Arb menu ([page 115](#)), press **Marker Utilities > Marker Polarity**.
2. For each marker, set the marker polarity as desired.
 - The default marker polarity is positive.
 - Each marker polarity is set independently.

See also, “[Saving Marker Polarity and Routing Settings](#)” on [page 111](#).

As shown on [page 120](#):

Positive Polarity: *On* marker points are high ($\approx 3.3V$).


Negative Polarity: *On* marker points are low (0V).

RF blanking always occurs on the low part of the signal regardless of the polarity setting.

Controlling Markers in a Waveform Sequence

In a waveform segment, an enabled marker point generates an auxiliary output signal that is routed to the rear-panel EVENT output (described in “Rear Panel Overview” on page 11) corresponding to that marker number. For a waveform sequence, you enable or disable markers on a segment-by-segment basis; this enables you to output markers for some segments in a sequence, but not for others. Unless you change the sequence marker settings or cycle the power, the marker setting for the last segment edited in the sequence applies to all segments in the next sequence that you build. For information on building a waveform sequence, see “Creating a Sequence” on page 102.

Figure 8-6 Waveform Sequence Menus for Enabling/Disabling Segment Markers

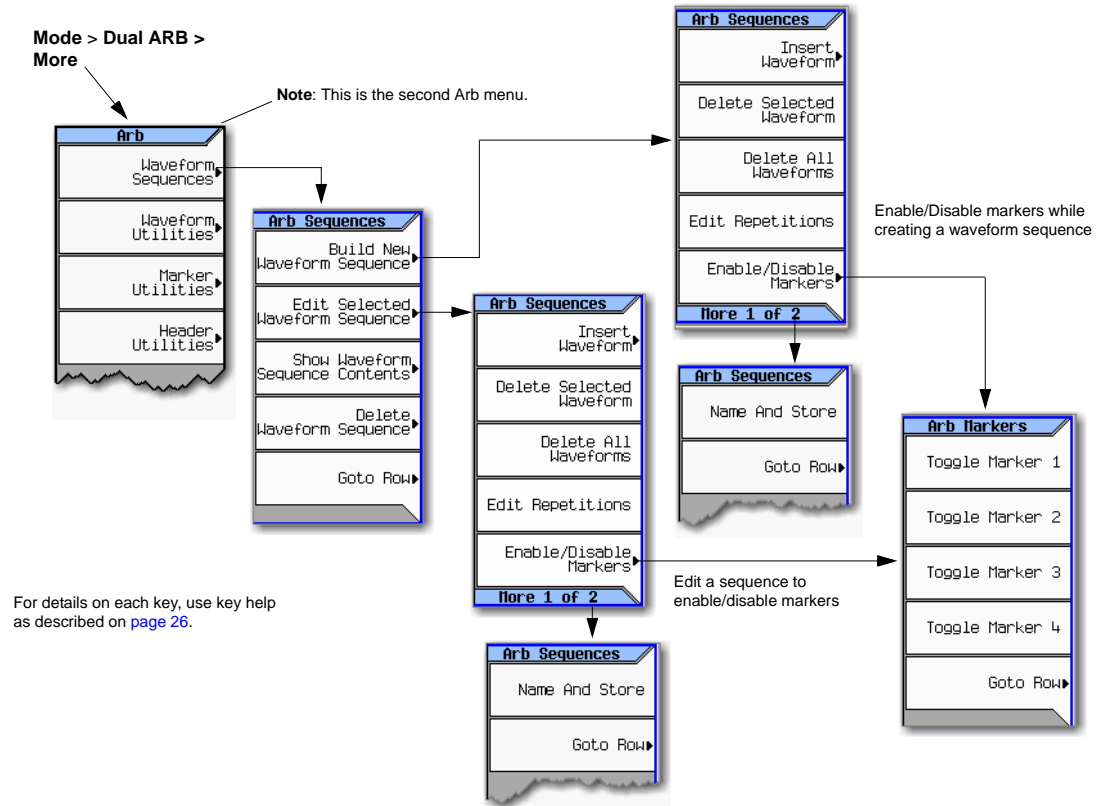

Enabling and Disabling Markers in a Waveform Sequence

Select the waveform segments within a waveform sequence to enable or disable each segment’s markers independently. You can enable or disable the markers either at the time of creating the sequence or after the sequence has been created and stored. If the sequence has already been stored, you must store the sequence again after making any changes. Enabling a marker that has no marker points has no effect on the auxiliary outputs. To set marker points on a segment, see “Setting Marker Points in a Waveform Segment” on page 117. This example assumes that a waveform sequence exists.

1. Ensure that all waveform segments for the sequence reside in BBG media (see page 98).
2. From the second Arb menu, press **Waveform Sequences**.
3. Highlight the desired waveform sequence.
4. Press **Edit Selected Waveform Sequence > Enable/Disable Markers**.
5. Toggle the markers:
 - a. Highlight the first waveform segment.
 - b. As desired, press **Toggle Marker 1**, **Toggle Marker 2**, **Toggle Marker 3**, and **Toggle Marker 4**.
An entry in the Mkr column (see figure below) indicates that the marker is enabled for that segment; no entry in the column means that all markers are disabled for that segment.
 - c. In turn, highlight each of the remaining segments and repeat **Step b**.
6. Press **Return > More > Name and Store**.
7. Either rename the sequence using the text entry keys (see page 99) or just press **Enter** to save the sequence with the existing name.

The markers are enabled or disabled per the selections, and the changes saved to the sequence file.

The following figure shows a sequence built using one of the factory-supplied waveform segments; a factory-supplied segment has a marker point on the first sample for all four markers. In this example, marker 1 is enabled for the first segment, marker 2 is enabled for the second segment, and markers 3 and 4 are enabled for the third segment.


Segment On BBG Media (1/1)	Sequence On Int. Media	(UNSTORED) (1/1)	Waveform	Reps	UNTITLED /tkr	Toggle Marker 4
RAMP_TEST_WFM	SEQ1	WF11:SINE_TEST_WFM	1	1		Sequence marker column
SINE_TEST_WFM	SINE100+RMP200	WF11:SINE_TEST_WFM	1	2		Toggle Marker 3
		WF11:SINE_TEST_WFM	1	3		This entry shows that markers 3 and 4 are enabled for this segment.

For each segment, only the markers enabled for that segment produce a rear-panel auxiliary output signal. In this example, the marker 1 auxiliary signal appears only for the first segment, because it is disabled for the remaining segments. The marker 2 auxiliary signal appears only for the second segment, and the marker 3 and 4 auxiliary signals appear only for the third segment.

Using the EVENT Output Signal as an Instrument Trigger

One of the uses for the EVENT output signal (marker signal) is to trigger a measurement instrument. You can set up the markers to start the measurement at the beginning of the waveform, at any single point in the waveform, or on multiple points in the waveform. To optimize the use of the EVENT signal for measurements, you may also need to adjust the sample rate. The location of the sample rate setting is shown in the figure at right.

For details on each key, use key help as described on [page 26](#).

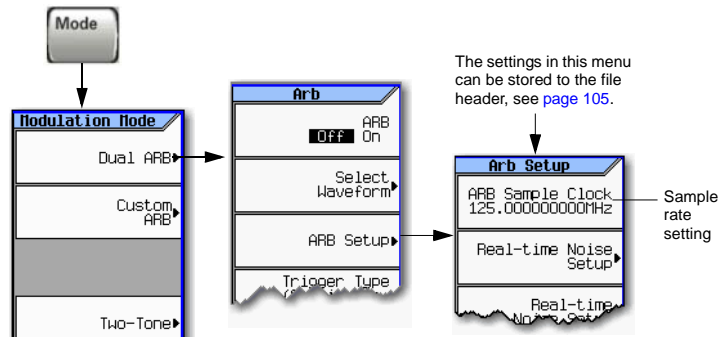

The EVENT output signal can exhibit jitter of up to ± 4 ns on the rising and falling edge. This jitter can be minimized in either of two ways.

Method 1: Use a sample clock of $125 \text{ MHz}/N$ where N is a positive integer and where $125 \text{ MHz}/N$ can be represented exactly on the display.

For example: 125 MHz, 62.5 MHz, 31.25 MHz, 25 MHz, and so on.


If the result cannot be represented exactly on the display, jitter will be present.

For example: $N = 6$ will result in jitter, because $125 \text{ MHz}/6 = 20.833 \text{ Mhz}$, which is truncated when displayed.

Method 2: Select a sample clock and waveform length that spaces the markers by a multiple of 8 ns. For example: A 200 point waveform with a marker on the first point and a sample clock of 50 MHz provides a marker every 4 μs . Because 4 μs is a multiple of 8 ns, the jitter is minimized.


When the EVENT output signal exhibits jitter and it is used as a measurement trigger, it can cause the waveform to falsely appear as having jitter. If this condition occurs, you can adjust the sample rate to a value (see above) that does not cause the jitter appearance. To maintain the integrity of the original waveform with a sample rate change, you will have to also recalculate the sample values. The following figures illustrate the marker signal jitter and its affect on the waveform.

EVENT output signal exhibits jitter due to a non-optimal sample rate

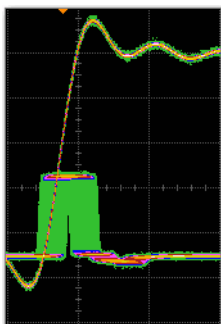


Oscilloscope triggering on waveform

Waveform appears to exhibit jitter when triggered using EVENT signal with jitter.

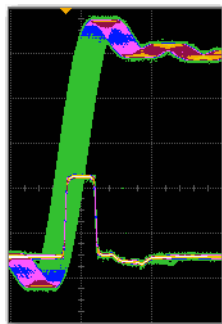

Oscilloscope triggering on EVENT signal

The jitter is gone with an optimal sample rate

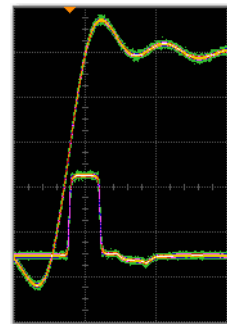


Oscilloscope triggering on EVENT signal

Triggering a Waveform

Figure 8-7 Triggering Softkeys

Mode > Dual ARB

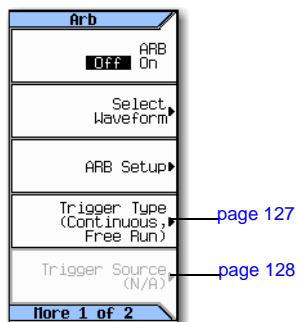

For details on each key, use key help as described on [page 26](#).

Triggers control data transmission by controlling when the signal generator transmits the modulating signal. You can configure trigger settings so that data transmission occurs once (Single mode), continuously (Continuous mode), or starts and stops repeatedly (Gated and Segment Advance modes).

A trigger signal contains both positive and negative states; you can use either for triggering.

When you initially select a trigger mode or when you change from one triggering mode to another, you may lose the carrier signal at the RF output until the modulating signal is triggered. This is because the signal generator sets the I and Q signals to zero volts prior to the first trigger event. To maintain the carrier signal at the RF output, create a data pattern with the initial I and Q voltages set to values other than zero.


When you initially turn the Arb ON or select a trigger mode or when you change from one triggering mode to another, you may temporarily lose the carrier signal for a few tens of milliseconds at the RF output. The Arb will present the idle IQrms value of the next Arb waveform to the IQ modulator. This ensures that the RF carrier output is at the correct amplitude level while the Arb waits for a trigger. When that trigger is received, the Arb begins playing the waveform and the modulated RF carrier exhibits no undesirable transients.

There are two parts to configuring a waveform trigger:

- *Type* determines the behavior of the waveform when it plays (see [Trigger Type](#) on page 127).
- *Source* determines how the signal generator receives the trigger that starts the modulating waveform playing (see [Trigger Source](#) on page 128).

Trigger Type

Type defines the trigger mode: how the waveform plays when triggered.

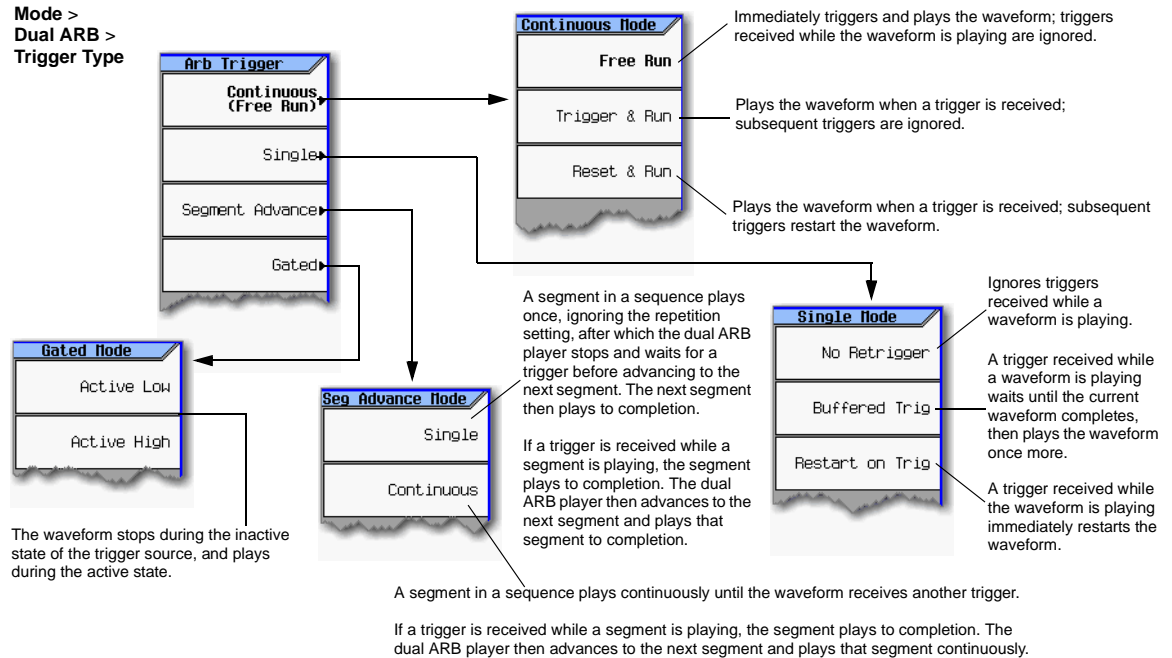


For details on each key, use key help as described on [page 26](#).

- **Continuous** mode repeats the waveform until you turn the signal off or select a different waveform, trigger mode, or response (Free Run, Trigger & Run, Reset & Run).
- **Single** mode plays the waveform once.
- **Segment Advance** mode plays a segment in a sequence only if triggered. The *trigger source* controls segment-to-segment playing (see [Example: Segment Advance Triggering](#) on page 129). A trigger received during the last segment loops play to the *first* segment in the sequence.
- **Gated** mode triggers the waveform at the first active triggering state, then repeatedly starts and stops playing the waveform in response to an externally applied gating signal. See [Example: Gated Triggering](#) on page 130.

Trigger Source

Mode >
Dual ARB >
Trigger Source

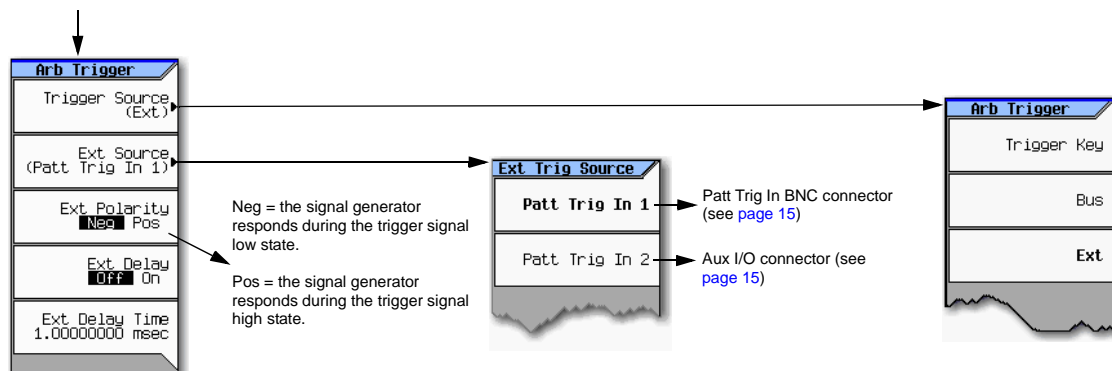

For details on each key, use key help as described on page 26.

External Trigger Polarity

- In Continuous, Single, and Segment Advance modes, use the **Ext Polarity** softkey to set the external trigger polarity.
- In Gated mode, the **Active Low** and **Active High** softkeys (page 127) determine the external trigger polarity.

Example: Segment Advance Triggering

Segment advance triggering enables you to control the segment playback within a waveform sequence. This type of triggering ignores the repetition value ([page 103](#)). For example if a segment has repetition value of 50 and you select Single as the segment advance triggering mode, the segment still plays only once. The following example uses a waveform sequence that has two segments.

If you have not created and stored a waveform sequence, refer to “[Creating a Sequence](#)” on [page 102](#).

1. Preset the signal generator.
2. Configure the RF output:
 - Set the desired frequency.
 - Set the desired amplitude.
 - Turn on the RF output.
3. Select a waveform sequence for playback:
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. In the Sequence On column, highlight a waveform sequence file.
 - c. Press **Select Waveform**.
4. Set the triggering as follows:
 - Trigger Type: continuous Segment Advance
Press **Trigger Type > Segment Advance > Continuous**.
 - Trigger source: Trigger hardkey
Press **Trigger Source > Trigger Key**.
5. Generate the waveform sequence:
Press **ARB Off On** until On highlights.
6. (Optional) Monitor the waveform:
Connect the RF OUTPUT of the signal generator to the input of an oscilloscope, and configure the oscilloscope so that you can see the signal.
7. Trigger the first waveform segment to begin playing continuously:
Press the **Trigger** hardkey.
8. Trigger the second segment:
Press the **Trigger** hardkey.


Pressing the **Trigger** hardkey causes the currently playing segment to finish and the next segment to start.

If the last segment in the sequence is playing, pressing the **Trigger** hardkey causes the *first* segment in the waveform sequence to start when the last segment finishes.

Example: Gated Triggering

Gated triggering enables you to define the on and off states of a modulating waveform.

1. Connect the output of a function generator to the signal generator's rear-panel PATT TRIG IN connector, as shown in the following figure. This connection is applicable to all external triggering methods. The optional oscilloscope connection enables you to see the effect that the trigger signal has on the RF output.

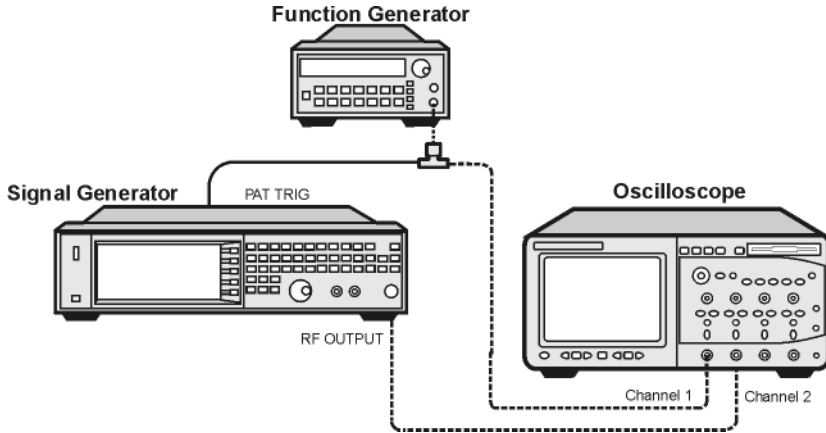


2. Preset the signal generator.
3. Configure the RF output:
 - Set the desired frequency.
 - Set the desired amplitude.
 - Turn on the RF output.
4. Select a waveform for playback (sequence or segment):
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. In the Segment On or Sequence On column, highlight a waveform.
 - c. Press **Select Waveform**.
5. Set the triggering as follows:
 - Trigger type: Gated
Press **Trigger Type > Gated**.
 - Active state: Low
Press **Active Low**.
 - Trigger source: External
Press **Trigger Source > Ext**.
 - Input connector: Rear panel Patt Trig In BNC
Press **Ext Source > Patt Trig In 1**.
6. Generate the waveform: Press **Return > ARB Off On** until On highlights.

7. On the function generator, configure a TTL signal for the external gating trigger.

8. (Optional) Monitor the waveform:


Configure the oscilloscope to display both the output of the signal generator, and the external triggering signal. You will see the waveform modulating the output during the gate *active* periods (low in this example).

The following figure shows an example display.

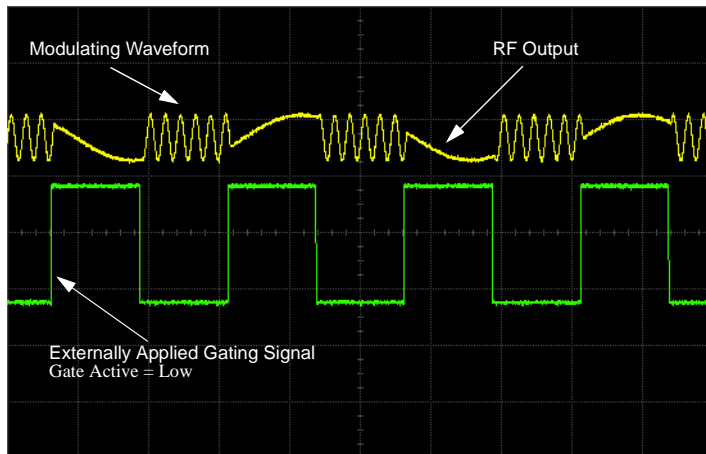

Example: External Triggering

Use the following example to set the signal generator to output a modulated RF signal 100 milliseconds after a change in TTL state from low to high occurs at the PATT TRIG IN rear panel BNC connector

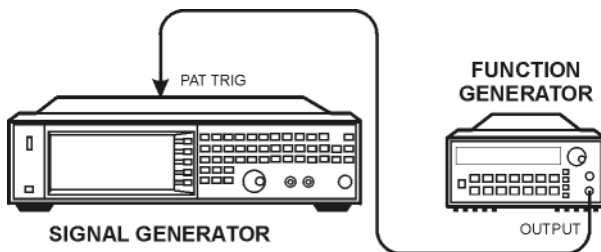


1. Connect the signal generator to the function generator as shown above.
2. Configure the RF output:
 - Set the desired frequency.
 - Set the desired amplitude.
 - Turn on the RF output.
3. Select a waveform for playback (sequence or segment):
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. In the Segment On or Sequence On column, highlight a waveform.
 - c. Press **Select Waveform**.
4. Generate the waveform:
Press **ARB Off On** until On highlights.
5. Set the waveform trigger as follows:
 - a. Trigger Type: single
Press **Trigger Type > Single > No Retrigger**
 - b. Trigger Source: external
Press **Trigger Source > Ext**
 - c. Input connector: Rear panel Patt Trig In BNC
Press **Ext Source > Patt Trig In 1**.
 - d. External Trigger Polarity: positive
Press **Ext Polarity** until Pos highlights
 - e. External Delay: 100 ms
Press **More > Ext Delay** until On highlights
Press **Ext Delay Time > 100 > msec**
6. Configure the Function Generator:
 - Waveform: 0.1 Hz square wave
 - Output Level: 3.5V to 5V.

Clipping a Waveform

Digitally modulated signals with high power peaks can cause intermodulation distortion, resulting in spectral regrowth that can interfere with signals in adjacent frequency bands. The clipping function enables you to reduce high power peaks by clipping the I and Q data to a selected percentage of its highest peak, thereby reducing spectral regrowth.

- [How Power Peaks Develop](#) on page 134
- [How Peaks Cause Spectral Regrowth](#) on page 136
- [How Clipping Reduces Peak-to-Average Power](#) on page 137
- [Configuring Circular Clipping](#) on page 140
- [Configuring Rectangular Clipping](#) on page 141

Figure 8-8 Clipping Softkeys

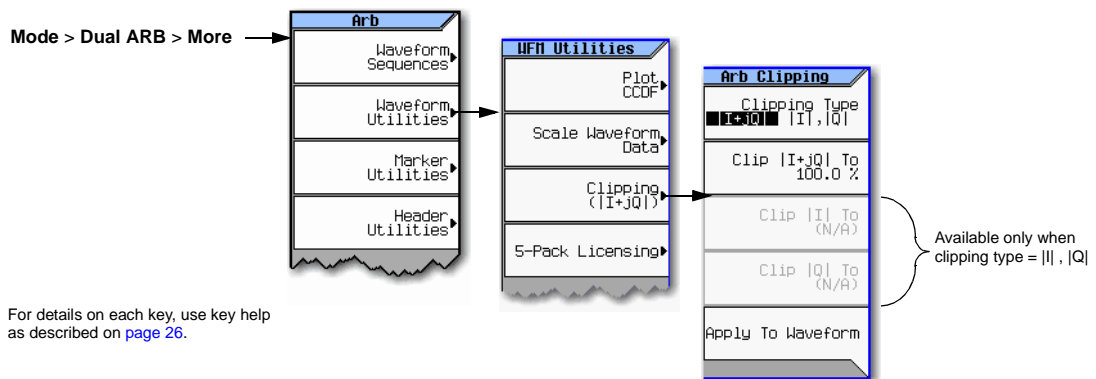


How Power Peaks Develop

To see how clipping reduces high power peaks, it is important to understand how the peaks develop as you construct a signal.

Multiple Channel Summing

I/Q waveforms can be the summation of multiple channels, as shown in the following figure. If a bit in the same state (high or low) occurs simultaneously in several individual channel waveforms, an unusually high power peak (positive or negative) occurs in the summed waveform.


Because the high and low states of the bits in channel waveforms are random and generally result in a cancelling effect, high power peaks occur infrequently with multiple channel summing.

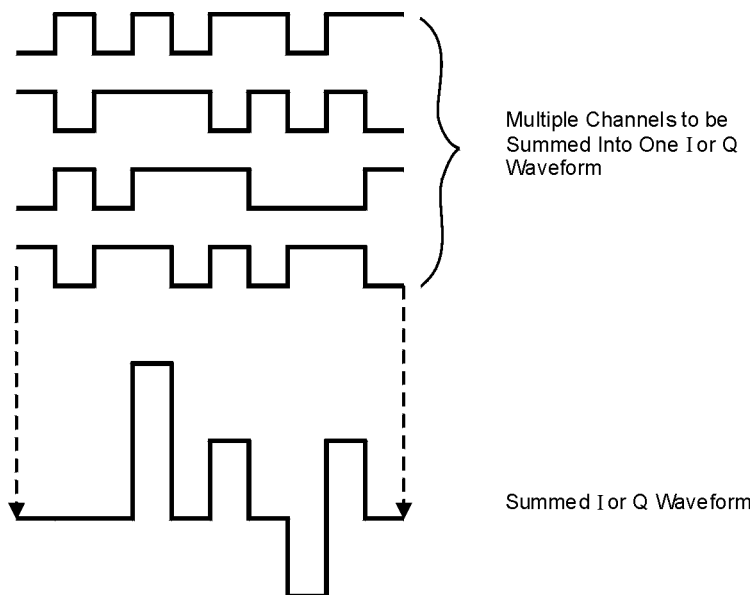

Combining the I and Q Waveforms


When the I and Q waveforms combine in the I/Q modulator to create an RF waveform, the magnitude of the RF envelope is $\sqrt{I^2+Q^2}$, where the squaring of I and Q always results in a positive value.

As shown in the following figure, simultaneous positive and negative peaks in the I and Q waveforms do not cancel each other, but combine to create an even greater peak.

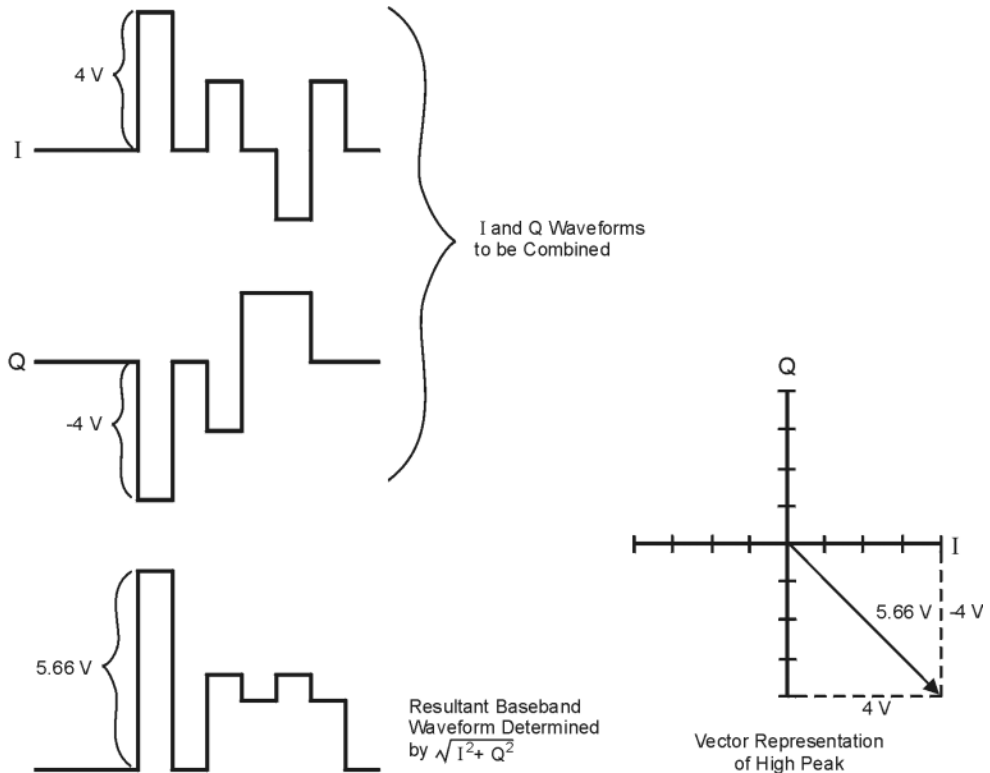


How Peaks Cause Spectral Regrowth

In a waveform, high power peaks that occur infrequently cause the waveform to have a high peak-to-average power ratio, as illustrated in the following figure.

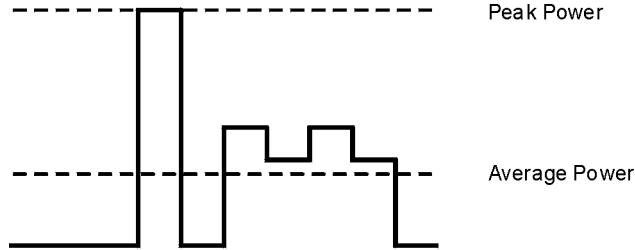

Because the gain of a transmitter's power amplifier is set to provide a specific average power, high peaks can cause the power amplifier to move toward saturation. This causes the intermodulation distortion that generates spectral regrowth. Spectral regrowth is a range of frequencies that develops on each side of the carrier (similar to sidebands) and extends into the adjacent frequency bands (see the following figure). Clipping provides a solution to this problem by reducing the peak-to-average power ratio.

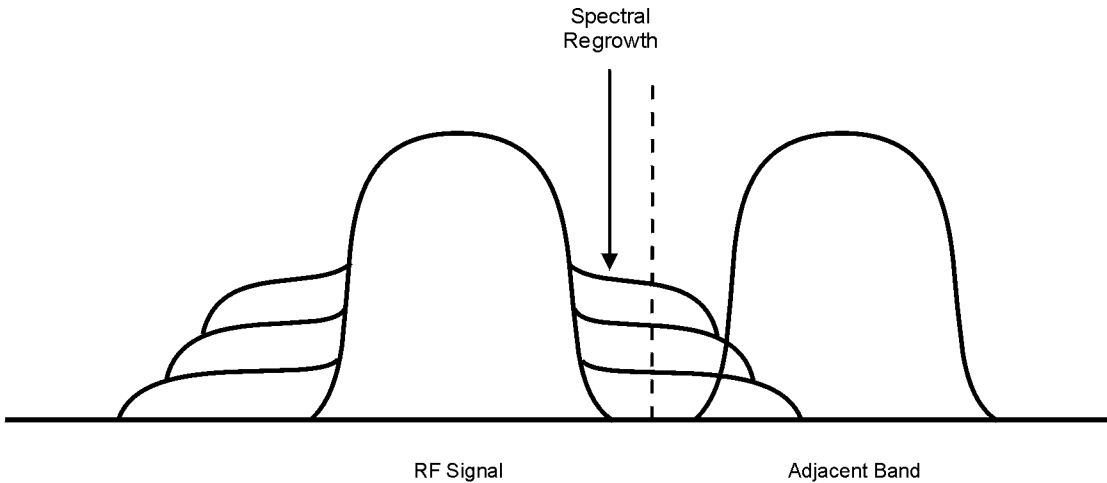

How Clipping Reduces Peak-to-Average Power

You can reduce peak-to-average power, and consequently spectral regrowth, by clipping the waveform. Clipping limits waveform power peaks by clipping the I and Q data to a selected percentage of its highest peak. The Signal Generator provides two methods of clipping:

- *Circular* clipping is applied to the composite I/Q data (I and Q data are equally clipped).

As shown in [Figure 8-9](#), the clipping level is constant for all phases of the vector and appears as a circle in the vector representation.

- *Rectangular* clipping is independently applied the I and Q data.

As shown in [Figure 8-10 on page 138](#), the clipping level is different for I and Q, and appears as a rectangle in the vector representation.

In both circular and rectangular clipping, the objective is to clip the waveform to a level that reduces spectral regrowth but does *not* compromise the integrity of the signal. The two complementary cumulative distribution plots in [Figure 8-11 on page 139](#) show the reduction in peak-to-average power that occurs after applying circular clipping to a waveform.

The lower the clipping value, the lower the peak power that is passed (the more the signal is clipped). The peaks can often be clipped without substantially interfering with the rest of the waveform. In many cases, data that might otherwise be lost in the clipping process is retained because of the error correction inherent in the coded systems. If you apply excessive clipping, however, lost data cannot be recovered. Experiment with clipping settings to find a percentage that reduces spectral regrowth while retaining needed data.

Figure 8-9 Circular Clipping

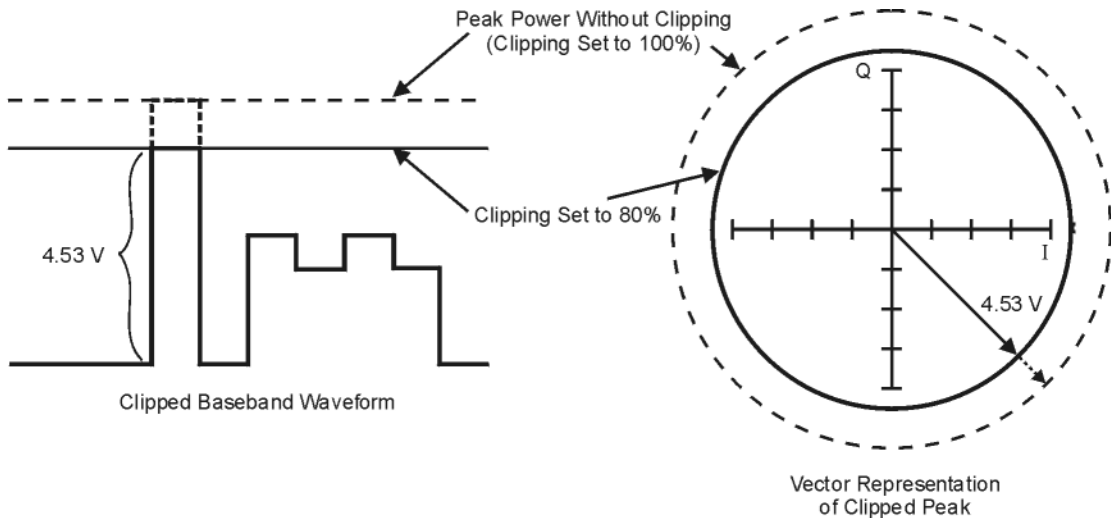


Figure 8-10 Rectangular Clipping


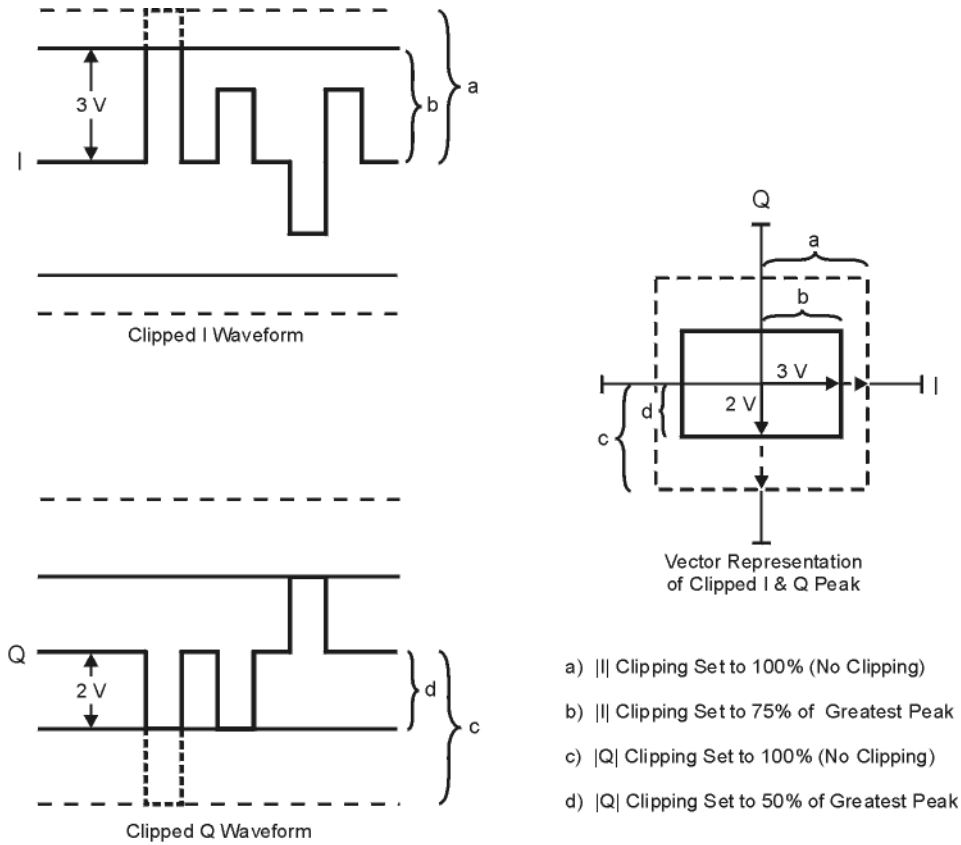


Figure 8-11 Reduction of Peak-to-Average Power

Complementary Cumulative Distribution

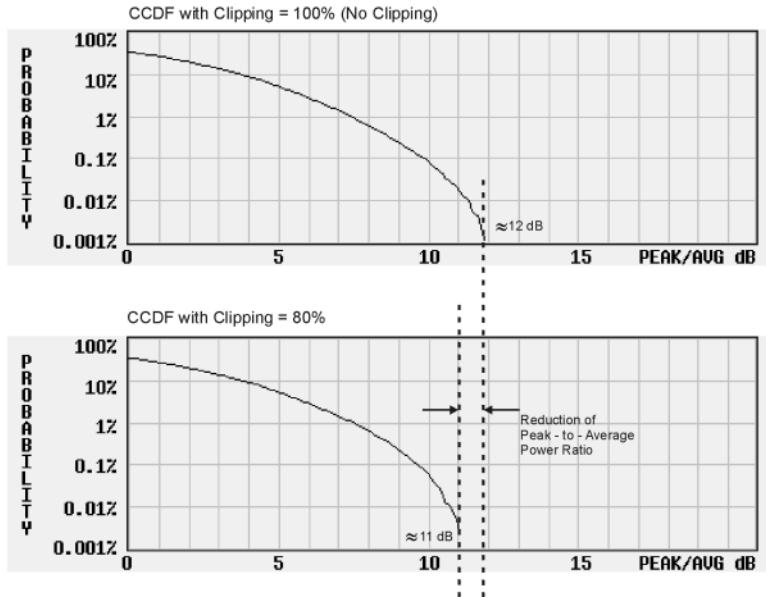

Configuring Circular Clipping

Use this example to configure circular clipping and observe its affect on the peak-to-average power ratio of a waveform. Circular clipping clips the composite I/Q data (I and Q data are clipped equally). For more information about circular clipping, refer to [“How Clipping Reduces Peak-to-Average Power” on page 137](#).

CAUTION Clipping is non-reversible and cumulative. Save a copy of the waveform file before you apply clipping.


Copy a Waveform File

1. Display the signal generator’s files: Press **File > Catalog Type > More > Volatile Segments**.
2. Highlight the waveform RAMP_TEST_WFM.
3. Press **Copy File**.
4. Name the copy (in this example, the name is MY_TEST_CIRC) and press **Enter**.

Apply Circular Clipping to the Copied Waveform File

1. Open the DUAL ARB Waveform Utilities menu: Press **Mode > Dual ARB > More > Waveform Utilities**.
2. In the list of files, highlight the copied file (in this example, MY_TEST_CIRC).

3. Create the CCDF plot: Press **Plot CCDF**.
4. Observe the shape and position of the waveform’s curve (the dark line in the example at right).

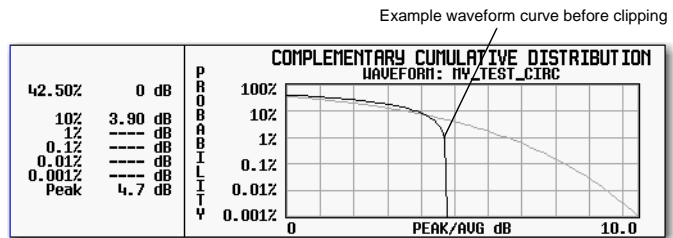


5. Activate circular clipping: Press **Return > Clipping > Clipping Type** until **|I+jQ|** highlights.

6. Set circular clipping to 80%:
Press **Clip |I+jQ| To > 80 > %**.

7. Apply 80% clipping to the I and Q data: Press **Apply to Waveform**.

8. Create the CCDF plot (see the example at right): Press **Plot CCDF**.

9. Observe the waveform’s curve after clipping.

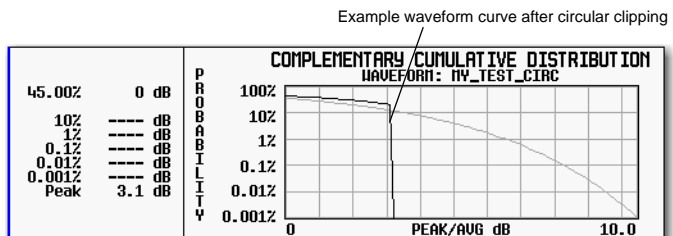

Note the reduction in peak-to-average power relative to the previous plot.

Configuring Rectangular Clipping

Use this example to configure rectangular clipping. Rectangular clipping clips the I and Q data independently. For more information about rectangular clipping, refer to [“How Clipping Reduces Peak-to-Average Power”](#) on page 137.

CAUTION Clipping is non-reversible and cumulative. Save a copy of the waveform file before you apply clipping.


Copy a Waveform File

1. Display the signal generator’s files: Press **File > Catalog Type > More > Volatile Segments**.
2. Highlight the waveform RAMP_TEST_WFM.
3. Press **Copy File**.
4. Name the copy (in this example, the name is MY_TEST_REC) and press **Enter**.

Apply Rectangular Clipping to the Copied Waveform File


1. Open the DUAL ARB Waveform Utilities menu: Press **Mode > Dual ARB > More > Waveform Utilities**.
2. In the list of files, highlight the copied file (in this example, MY_TEST_REC).
3. Create the CCDF plot: Press **Plot CCDF**.
4. Observe the shape and position of the waveform’s curve (the dark line in the example at right).
5. Activate rectangular clipping: Press **Return > Clipping > Clipping Type** until **|I|,|Q|** highlights.
6. Set 80% clipping for the I data: Press **Clip |I| To > 80 > %**.
7. Set 40% clipping for the Q data: Press **Clip |Q| To > 40 > %**.
8. Apply the rectangular clipping to the waveform: Press **Apply to Waveform**.

Example waveform curve before clipping

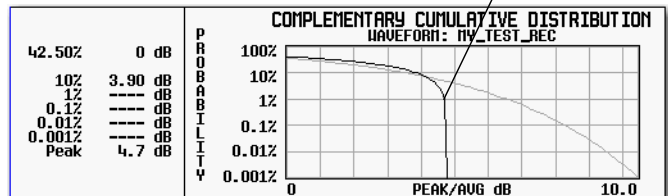

9. Create the CCDF plot (see the example at right): Press **Plot CCDF**.
10. Observe the waveform’s curve after clipping.
Note the reduction in peak-to-average power relative to the previous plot.

Example waveform curve after rectangular clipping

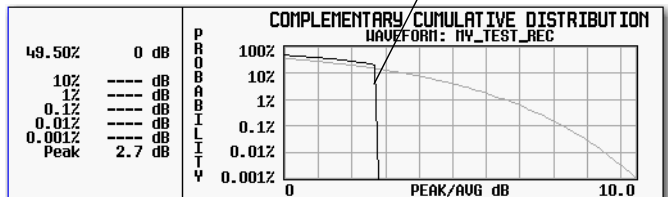


Scaling a Waveform

The signal generator uses an interpolation algorithm (sampling between the I/Q data points) when reconstructing a waveform. For common waveforms, this interpolation can cause overshoots, which may create a DAC over-range error condition. This chapter describes how DAC over-range errors occur and how you can use waveform scaling to eliminate these errors.

- [How DAC Over-Range Errors Occur](#) on page 144
- [How Scaling Eliminates DAC Over-Range Errors](#) on page 145
- Agilent MXG waveform scaling on [page 146](#) and [page 147](#):
 - Waveform runtime scaling to scale a currently-playing waveform
 - Waveform scaling to permanently scale either the currently playing waveform, or a non-playing waveform file in BBG media


Figure 8-12 Scaling Softkeys

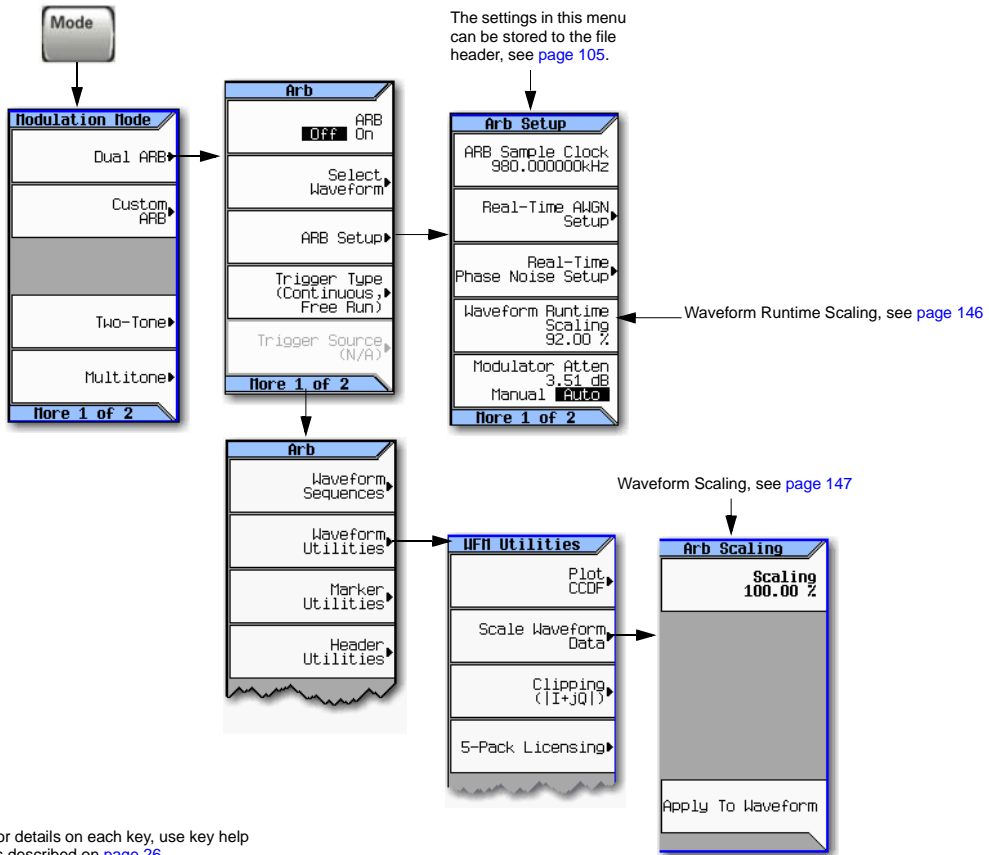


For details on each key, use key help as described on page 26.

How DAC Over-Range Errors Occur

The signal generator uses an interpolator filter when it converts digital I and Q baseband waveforms to analog waveforms. Because the clock rate of the interpolator is four times that of the baseband clock, the interpolator calculates sample points between the incoming baseband samples and smooths the waveform as shown in the figure at the right.

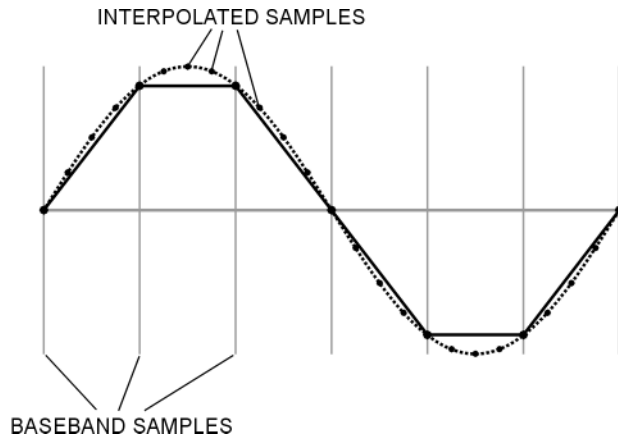


The interpolation filters in the DACs overshoot the baseband waveform. If a baseband waveform has a fast-rising edge, the interpolator filter's overshoot becomes a component of the interpolated baseband waveform. This response causes a ripple or ringing effect at the peak of the rising edge. If this ripple overshoots the upper limit of the DAC range, the interpolator calculates erroneous sample points and is unable to replicate the true form of the ripple (see the figure at the right). As a result, the signal generator reports a DAC over-range error.

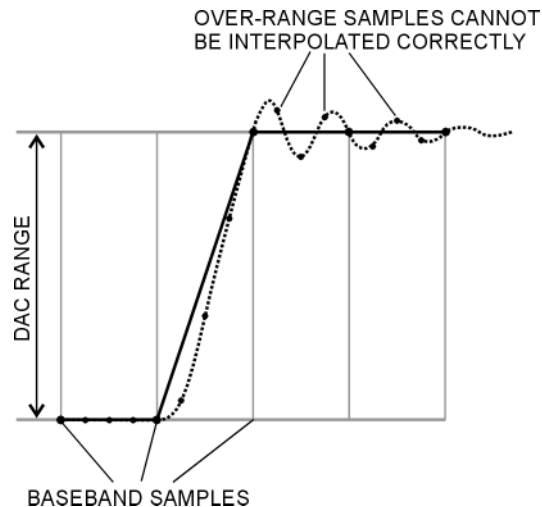

How Scaling Eliminates DAC Over-Range Errors

Scaling reduces the amplitude of the baseband waveform while maintaining its basic shape and characteristics, such as peak-to-average power ratio. If the fast-rising baseband waveform is scaled enough to allow an adequate margin for the interpolator filter overshoot, the interpolator filter can calculate sample points that include the ripple effect and eliminate the over-range error (see the figure at the right).

Although scaling maintains the basic shape of the waveform, excessive scaling can compromise waveform integrity. For example, if the bit resolution becomes too low the waveform becomes corrupted with quantization noise. To achieve maximum accuracy and optimize dynamic range, scale the waveform no more than is required to remove the DAC over-range error. Optimum scaling varies with waveform content.

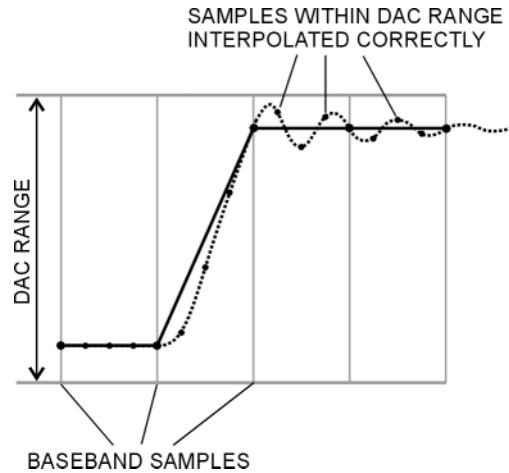

Setting Waveform Runtime Scaling

Runtime scaling scales the waveform data during playback; it does not affect the stored data. You can apply runtime scaling to either a segment or sequence, and set the scaling value either while the ARB is on or off. This type of scaling is well suited for eliminating DAC over-range errors. Runtime scaling adjustments are not cumulative; the scaling value is applied to the original amplitude of the waveform file. There are two ways to save the runtime scaling setting: by using the save function (page 52) and by saving the setting to the file header (page 107). Saving to the file header saves the value with the waveform file, saving with the Save function stores the value as the current instrument setting.

Use this example to learn how to scale the currently selected waveform.

1. Select the waveform to which you want to apply scaling:
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. Highlight the desired waveform (segment or sequence).
 - c. Press **Select Waveform**.
2. Play the selected waveform: Press **ARB Off On** until On highlights.
3. Set the Waveform Runtime Scaling value:
 - a. Press **ARB Setup > Waveform Runtime Scaling**.
 - b. Enter a scaling value.

The signal generator automatically applies the new scaling value to the waveform. There is no single value that is optimal for all waveforms. To achieve the maximum dynamic range, use the largest scaling value that does not result in a DAC over-range error.


- c. Press **Return**.

Setting Waveform Scaling

Waveform scaling differs from waveform runtime scaling in that it permanently affects waveform data and only applies to waveform segments stored in BBG media. You scale the waveform either up or down as a percentage of the DAC full scale (100%). If you scale your waveforms using this method, you may also need to change the waveform runtime scaling value to accommodate this scaling.

When you scale, the signal generator permanently modifies the waveform file's sample values so that they conform to the desired scaling value. When you initiate scaling, the signal generator performs the following actions:

- locates the waveform file's absolute peak sample value
- determines its current percentage of full scale
- calculates the ratio of the desired scale value to the determined absolute peak sample scale value
- multiplies each sample in the waveform file by this ratio

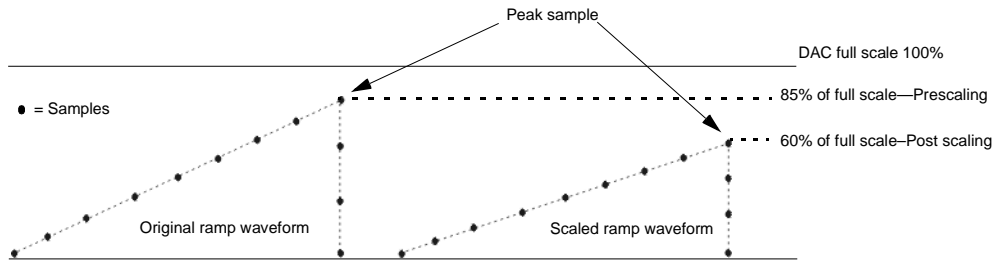

Scaled sample value = scaling ratio × prescale sample val

Scaling ratio = desired scale val / current scale val
 = 60 / 85
 = 0.70588

Each sample in the waveform is multiplied by 0.70588 to reach the 60% post scaling waveform amplitude.

When you scale a waveform, you can create fractional data, lose data, or both. Fractional data occurs almost every time you reduce or increase the scaling value, and causes quantization errors.

Quantization errors are more noticeable when scaling down, since you are closer to the noise floor. You lose data when either the signal generator rounds fractional data down or the scaling value is derived using the results from a power of two. This means that scaling a waveform in half (power of two: $2^1 = 2$) causes each waveform sample to lose one bit. The waveform data modifications are not correctable and may cause waveform distortion. It is always best to make a copy of the original file prior to applying scaling.

Use the following examples to apply waveform scaling to a waveform file. While this process uses the factory-supplied waveform `RAMP_TEST_WFM`, it is the same for any waveform file.

Copy a Waveform File

1. Display the waveform files in BBG media: Press **File** > **Catalog Type** > **More** > **Volatile Segments**.
2. Highlight the waveform `RAMP_TEST_WFM`.
3. Press **Copy File**.
4. Name the copy (this example uses the name `MY_TEST_SCAL`) and press **Enter**.

Apply Scaling to the Copied Waveform File


CAUTION This type of scaling is non-reversible. Any data lost in the scaling operation cannot be restored. Save a copy of the waveform file before scaling.

1. Open the DUAL ARB Waveform Utilities menu:
Press **Mode > Dual ARB > More > Waveform Utilities**.
2. In the list of BBG Media segment files, highlight the copied file (in this example, MY_TEST_SCAL).
3. Set and apply a scaling value (in this example 70% scaling is applied):
Press **Scale Waveform Data > Scaling > 70 > % > Apply to Waveform**.

Setting the Baseband Frequency Offset

The baseband frequency offset enables you to shift the baseband frequency up to ± 50 MHz within the BBG 100 MHz signal bandwidth, depending on the signal generator's baseband generator option. While the following figure shows how to access the control using the Dual ARB player, the location of the **Baseband Frequency Offset** softkey within each arb format, through the **ARB Setup** softkey, is the same as for the Dual ARB player.

Figure 8-13 Baseband Frequency Offset Softkey for the Dual ARB Player

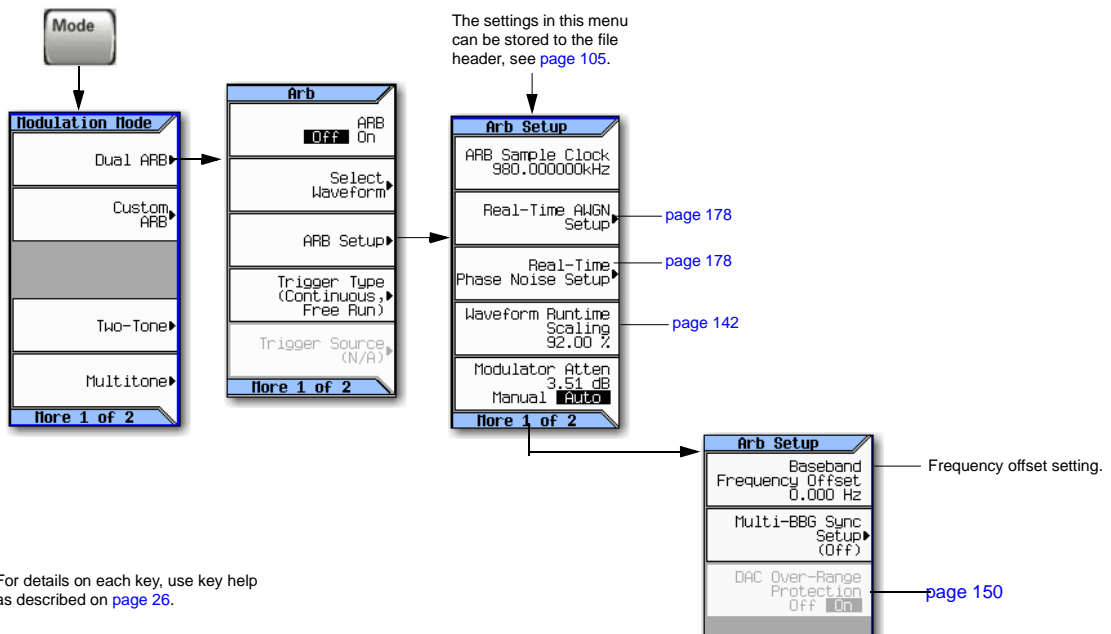

Common uses for the offset feature include:

- offsetting the carrier from any LO feedthrough (carrier signal spur at the carrier frequency)
- sum the baseband signal with external I and Q inputs to create a multicarrier signal
- use the signal generator's I/Q signal as an IF

NOTE Changing the baseband frequency offset may cause a DAC over range condition that generates error 628, Baseband Generator DAC over range. The signal generator incorporates an automatic scaling feature to minimize this occurrence. For more information, see “DAC Over-Range Conditions and Scaling” on [page 150](#).

The baseband frequency offset value is one of the file header parameters ([page 105](#)), which means you can store this value with the waveform. When you select a waveform with a stored frequency offset value, the signal generator changes the current value to match the stored file header value. If there is no stored baseband offset frequency value for the current waveform, the signal generator uses the last set frequency offset value.


You can also use the Save function ([page 52](#)) to store this value as part of the signal generator setup.

When you Recall a setup stored with the Save function, the baseband frequency offset value becomes the current instrument setting value, disregarding the stored file header value.

Use the following steps to offset the carrier from LO/carrier feedthrough. This example uses the factory supplied waveform, SINE_TEST_WFM available in the Dual ARB Player. To view the output for this example, connect the RF OUTPUT of the signal generator to the input of a spectrum analyzer.

1. Select and play the waveform.
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. In the Segment On BBG Media column, select SINE_TEST_WFM.
 - c. Press **Select Waveform**.
2. Generate the waveform: Press **ARB Off On** to On.
3. Configure the carrier signal:
 - a. Set the carrier signal to 1 GHz.
 - b. Set the amplitude to 0 dBm.
 - c. Turn on the RF OUTPUT.
4. Press **ARB Setup > Baseband Frequency Offset > 20 MHz**.

The modulated RF signal is now offset from the carrier frequency by 20 MHz as shown in the following figures.

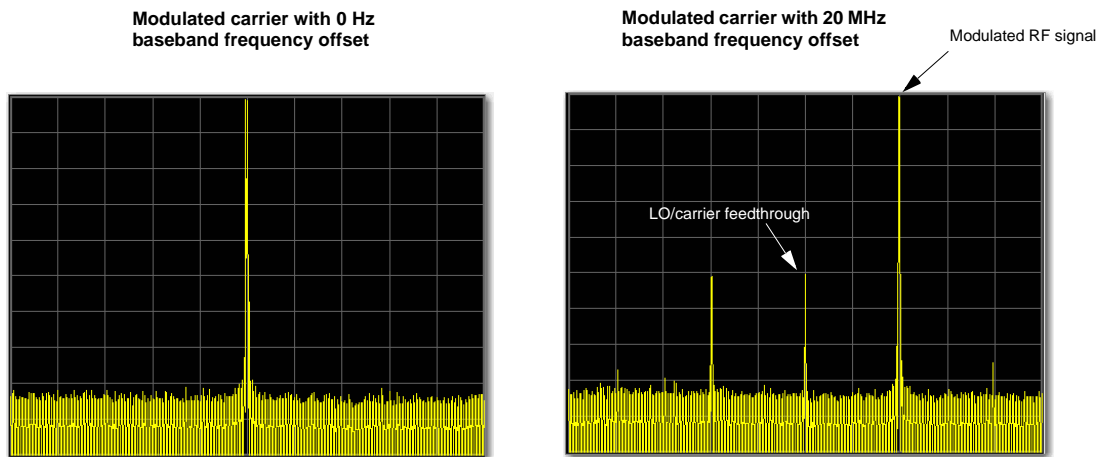

Spectrum analyzer set to a span of 100 MHz


DAC Over-Range Conditions and Scaling

When using the baseband frequency offset (at a setting other than 0 Hz), it is possible to create a DAC over-range condition, which causes the Agilent MXG to generate an error. To minimize this condition with the frequency offset feature, the Agilent MXG incorporates an automatic DAC over-range protection feature that scales down the I/Q data by $1/\text{square root of } 2$ when the offset is something other than zero. Because it can scale the data by more than what is actually need, it

typically decreases the dynamic range of the waveform. This is especially noticeable when using a constant amplitude signal such as GSM.

For the Dual ARB Player, this automatic over-range feature can be turned off. When on, it is active for the Dual ARB signal only when the offset is something other than 0 Hz. The control for the Dual ARB DAC over-range protection feature is located in the key path as shown in [Figure 8-14](#).

Figure 8-14 Dual ARB DAC Over-Range Protection Softkey Location

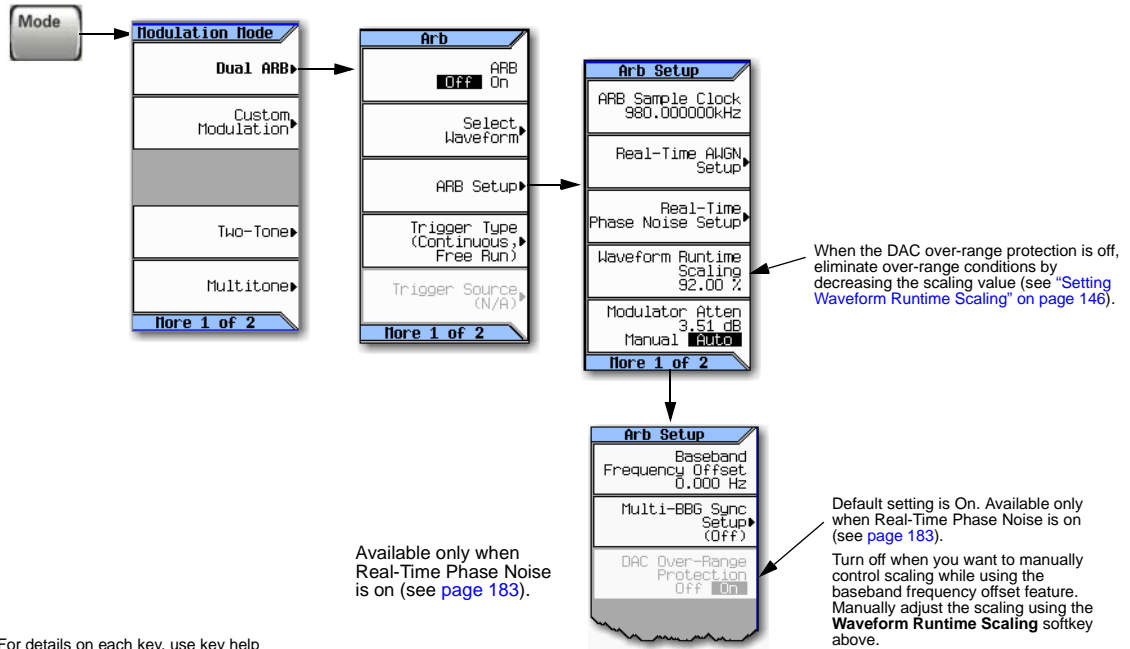

For details on each key, use key help as described on [page 26](#).

In the Dual ARB Player, to avoid excessive scaling or to just perform scaling manually, turn the feature off and use the **Waveform Runtime Scaling** softkey to eliminate DAC over-range conditions.

I/Q Modulation


The following factors contribute to the error vector magnitude:

- Differences in amplitude, phase, and delay between the I and Q channels
- DC offsets

The I/Q menu not only enables you to select the I/Q signal source and output, it also provides adjustments and calibrations to compensate for differences in the I and Q signals.

See also, “Modulating the Carrier Signal” on page 43.

Figure 8-15 I/Q Display and Softkeys

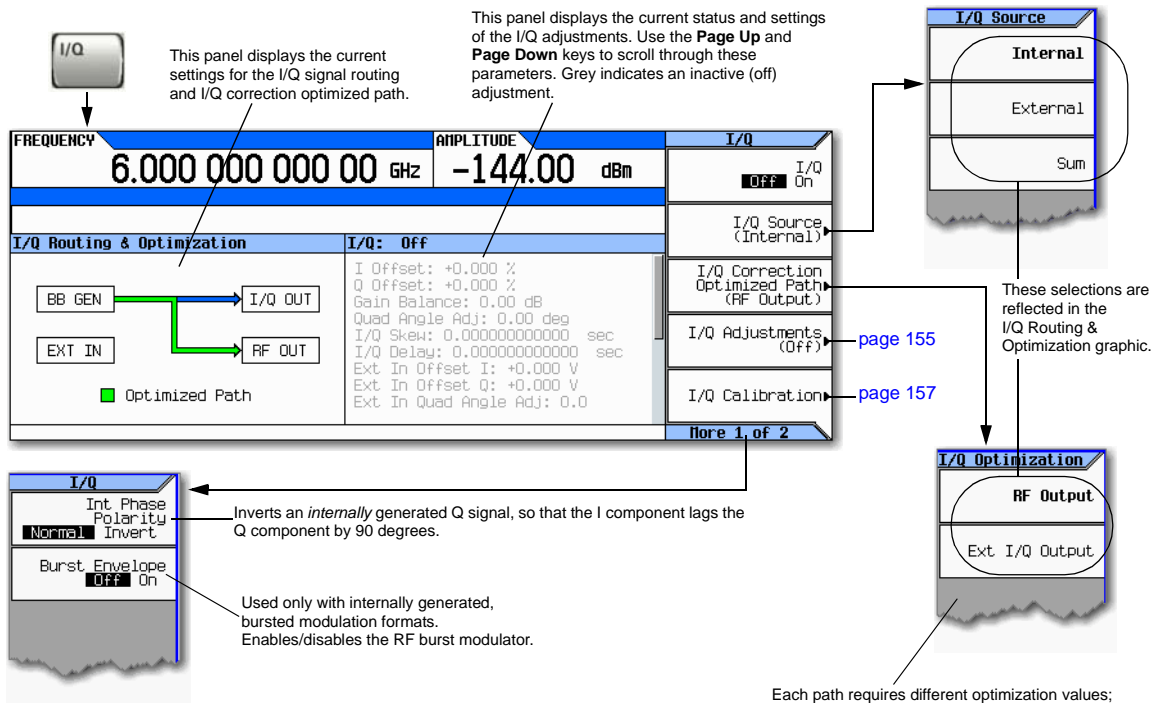

For details on each key, use key help as described on page 26.

Each path requires different optimization values; when you select a path, you are selecting the unique optimization values required by that path. The signal generator applies the selected optimization values to both paths, which impairs the unselected path.

Using the Rear Panel I and Q Outputs

NOTE The rear-panel I and Q connectors only output a signal while using the internal BBG.

In addition to modulating the carrier, the signal generator also routes the internally generated I and Q signals to the rear panel I and Q connectors. These output signals are post DAC, so they are in analog form. You can use these rear panel I and Q signals to:

- drive a system's transmitter stage
- test individual analog I and Q components such as an I/Q modulator
- route the I and Q signals into another signal generator

The factory default setting routes the internally generated I and Q signals to the I/Q modulator and the rear panel I and Q output connectors. However to optimize (apply calibration factors) the rear panel signals, you need to select the external I/Q output path.

Select and Play a Waveform

1. Press **Mode > Dual ARB > Select Waveform**.
2. Highlight the desired waveform.
3. Press **Select Waveform > ARB Off On to On**.

Optimize the Signal Path


1. Connect cables from the rear panel I and Q connectors to either a DUT or another signal generator.

When you turn the ARB on, the signal generator automatically outputs the I and Q signals to the rear panel connectors. You can use the rear panel I and Q signals as I and Q inputs to another signal generator. The MXG has front panel connectors, I Input and Q Input, for this purpose.



2. Press **I/Q > I/Q Correction Optimized Path > Ext I/Q Output**.

When you optimize a path, the path indicator turns green.

Factory default setting—RF Output path optimized

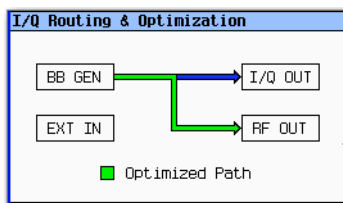

Rear-panel I/Q path optimized

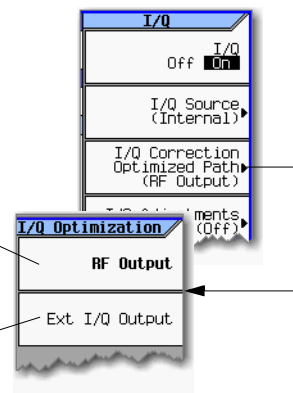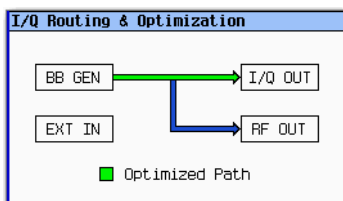

Configuring the Front Panel Inputs

The signal generator accepts externally supplied analog I and Q signals through the front-panel I Input and Q Input. You can use the external signals as the modulating source, or sum the external signals with the internal baseband generator signals.


1. Connect I and Q signals to the front panel connectors.
 - a. Connect an analog I signal to the signal generator's front-panel I Input.
 - b. Connect an analog Q signal to the signal generator's front-panel Q Input.
2. Set the signal generator to recognize the front-panel input signals:

- **To Modulate onto the Carrier**

Press **I/Q > I/Q Source > External**.

Signal generator display: both paths are calibrated when the **I/Q Correction Optimized Path** is set to **Ext I/Q Output** (see [page 153](#))

Note: when the optimized path is set to RF, *only* the RF Out path is calibrated.

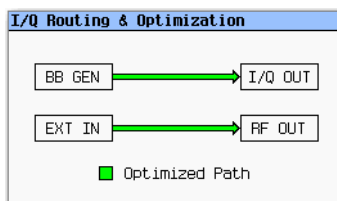


- **To Sum and Modulate onto the Carrier**

Press **I/Q > I/Q Source > Sum**.

To select and play a waveform for the BB GEN path, see [page 99](#).

Signal generator display: both RF paths are calibrated when the **I/Q Correction Optimized Path** is set to **RF Output** (see [page 153](#))

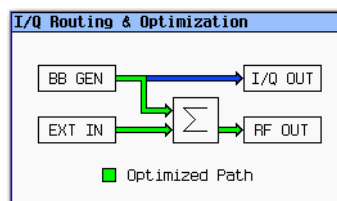




Notice that only the internal BBG (BB GEN) routes I and Q signals to the rear-panel I and Q outputs.

3. If you are using only the external I and Q signals (no summing), turn on the I/Q modulator: Press **I/Q Off On** to On.
4. Configure the RF output:
 - a. Set the carrier frequency.
 - b. Set the carrier amplitude.
 - c. Turn the RF output on.

I/Q Adjustments

Use the I/Q Adjustments to compensate for or add impairments to the I/Q signal.

I/Q > I/Q Adjustments

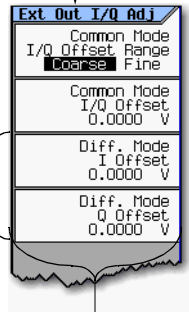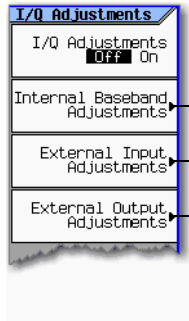

Available only with Option 1EL

Offsets are typically used to either reduce carrier leakage, or to create an impairment that simulates carrier leakage.

Common Mode I/Q Offset Range
This changes the adjustment range of the Common Mode I/Q Offset from Coarse (Default) to fine or vice versa. The Coarse range corresponds to the default value of $\pm 2.5V$. The Fine range corresponds to a value of ± 100 mV.

Common Mode I/Q Offset
This adjusts the DC offset of both I and Q signals simultaneously.

Diff Mode I Offset
This adjusts the DC offset level of the I and I-bar output signal. I and I-bar cannot be adjusted independently.

Diff Mode Q Offset
This adjusts the DC offset level of the I and I-bar output signal. I and I-bar cannot be adjusted independently.

The DC offset values are calibrated relative to the RMS waveform voltage being played out of the ARB. See page 107.



Adjusts the I signal amplitude relative to the Q signal amplitude. Use this as an internal impairment, or to compensate for differences in signal path loss that occur due to path irregularities in the external I and Q output cabling.

Offsets the phase of the Q signal relative to the phase of the I signal. The baseband quadrature adjustment key is calibrated in units of degrees. The external input quadrature adjustment is not calibrated. The function provided by this key is not the same as the function provided by the I/Q Skew key.

Skew is typically used either to create impairments, or to reduce error vectors on large bandwidth signals.

Provides a relative time delay correction between the I and Q signals. The different signal paths traveled by the I and Q signals result in time delay differences that show up as an EVM error in large bandwidth modulated signals.

Adding an equal and opposite time delay (skew) in the I/Q signals during baseband generation eliminates the time delay error, correcting for any delays in signals that are generated in the internal baseband generator.

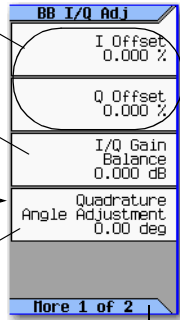

Available only when a waveform is playing.

Changes the absolute phase of both the I and Q signals with respect to triggers and markers.

Positive values add delay and negative values advance the signals. This value affects both the baseband signal modulated onto the RF and the external output signals (I and Q). This setting cannot be used with constant envelope modulation and it does not affect external I and Q inputs.

Table 8-2 I/Q Adjustments Uses

I/Q Adjustment	Effect	Impairment
Offset	Carrier feedthrough	dc offset
Quadrature Angle	EVM error	phase skew
	I/Q Images	I/Q path delay
I/Q Skew	EVM error	high sample rate phase skew or I/Q path delay
I/Q Gain Balance	I/Q amplitude difference	I/Q gain ratio

The I/Q adjustment, I/Q Delay, is not for adding impairments; its function is to compensate for any latency between the EVENT output signals (marker signals) and the RF output.


I/Q Calibration

Use the I/Q calibration for I and Q signal corrections. What aspects of the I and Q signal is corrected depends on whether the signal is internally or externally generated.

Correction	Internal I and Q	External I and Q
Offset	X	X
Gain Balance	X	--
Quadrature Error	X	X

When you perform an I/Q calibration, that calibration data takes precedence over the factory-supplied calibration data. The calibration routines improves performance that may degrade over time or due to temperature changes.

I/Q > I/Q Calibration

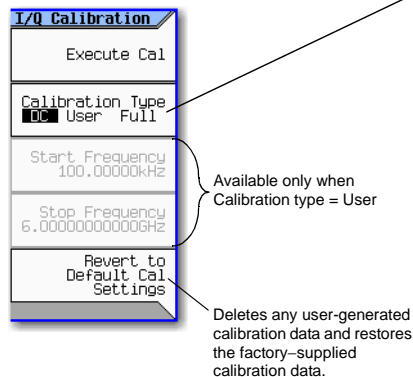

DC optimizes the I/Q performance for the current instrument settings, and typically completes in several seconds. Changing any instrument setting except for I/Q adjustments after performing a DC calibration voids the DC calibration and causes the signal generator to revert to the factory-supplied calibration data.

Presetting the instrument or cycling power is equivalent to pressing **Revert to Default Cal Setting**.

User provides a quicker calibration when a full calibration is not required. You can limit the calibration by specifying the calibration start and stop frequencies.

When you limit the calibration to less than the instrument's full frequency range, the factory-supplied calibration data is used for the rest of the range.

Information is retained through a preset or power cycle.

Full takes 5 minutes, executing measurements over the instrument's entire frequency range.

Information is retained through a preset or power cycle.

Note

A DC calibration requires the following settings:

- I/Q: On
- Optimized Path: RF Output
- Source: Internal


For details on each key, use key help as described on [page 26](#).

Multiple Baseband Generator Synchronization

Available in the Dual ARB menu, this feature lets you set up a master/slave system of up to sixteen Agilent MXGs so that the baseband generators (BBG) synchronize the playing of waveforms. The system count includes one Agilent MXG to function as the master (see “Equipment Setup” on page 161).

Figure 8-16 Multiple Baseband Generator Synchronization (BBG Synchronization) Trigger Softkeys and Menu Location

Note: The BBG sync feature automatically configures the trigger settings shown below. To avoid a settings conflict error in this process, manually configure the trigger settings prior to setting the BBG sync parameters shown on page 159.

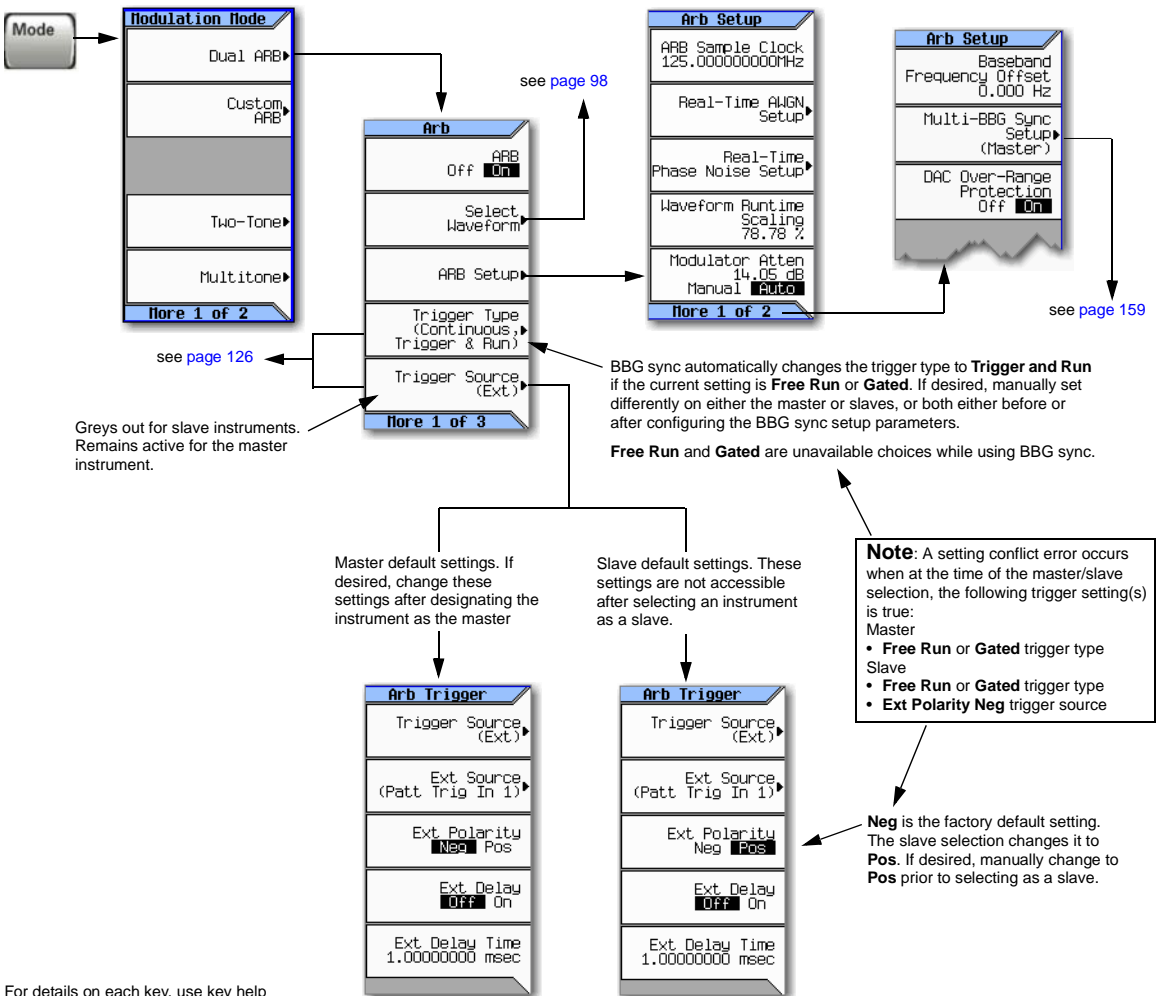

For details on each key, use key help as described on page 26.

Figure 8-17 Multiple BBG Synchronization Front Panel Displays

Master Display and Available Softkeys

Select Off, Master, or Slave

This is a persistent setting that survives both preset and cycling the power.

Grayed-out on master, active for slaves.

Synchronizes the baseband generators for all instruments in the system.

Note: Press only after pressing Listen for Sync on all slave instruments and the slaves show "Waiting For Sync" as the status.

Master shows one of the following messages:

- Out of Sync
- In Sync

Shows after pressing Sync Slaves

Master/slave indicator and setup diagram.

Slave Display and Available Softkeys

Select Off, Master, or Slave

These are persistent settings that survive both preset and cycling the power.

After pressing, the slave waits for the synchronization signal initiated by the master.

Note: Press before pressing Sync Slaves on the master instrument.

Slave shows one of the following messages:

- Out of Sync
- Waiting for Sync
- In Sync

Shows after pressing Listen for Sync

Shows after pressing Sync Slaves on the master

Master/slave indicator and setup diagram. The bottom slave indicator is green on the last slave in the system.

For details on each key, use key help as described on page 26.

Understanding the Master/Slave System

System Delay

The multiple BBG synchronization feature provides a system for synchronizing the waveform generation capability of up to 16 signal generators to within a characteristic value of ± 8 ns between the master and the last slave. This minor amount of delay (± 8 ns) can be reduced further to picosecond resolution by using the **I/Q Delay** softkey located in the **I/Q** menu. To reduce the delay, check and adjust the BBG signal alignment for each signal generator in the system. For more information on adjusting the delay, see [“I/Q Adjustments” on page 155](#).

The delay value includes compensation for cables that have less than 1 ns of propagation delay between the **EVENT 1** and **PAT TRIG** connectors (see [Equipment Setup](#)). The recommended cable is an Agilent BNC cable, part number 10502A. The use of cables with greater propagation delay may not allow the signal generators to properly synchronize.

System Synchronization

Synchronization occurs after the master signal generator sends a one-time event pulse that propagates through and to each slave in the system. Prior to this event, each slave must recognize that it is waiting for this event pulse, which occurs during the system configuration (see [“Configuring the Setup” on page 161](#)). In order to properly send the synchronization pulse, the trigger source and the Dual ARB Player for each signal generator must be turned off.

The master/slave setup does *not* incorporate a feedback system between the slaves and the signal generator selected as the master. After synchronization, if changes occur to the Multi-BBG Sync Setup menu or a signal generator is added to the system, the master does not automatically resynchronize the setup. This may cause the signal generators in the system to incorrectly report their status as In Sync.

The system can also misinterpret other signals as the synchronization pulse, which results in an incorrect In Sync status. These types of signals include a continuous trigger or an active Marker routed to the EVENT 1 connector. Improperly connected rear-panel cables can also create a false status.

You must resynchronize the entire system after making any change in one or all of the Multi-BBG Sync Setup menus, after adding a signal generator to the system, or in doubt as to the true status of a signal generator. Changes to parameters that are outside of the Multi-BBG Sync Setup menu such as waveform files, Dual ARB state, sample rate, scaling, carrier frequency or amplitude have no effect on the system synchronization. To resynchronize a system, see [“Making Changes to the Multiple Sync Setup and Resynchronizing the Master/Slave System” on page 163](#).

System Trigger Setup

The multiple BBG synchronization feature restricts the trigger selections (see [page 158](#)) for each signal generator. For signal generators selected as slaves, you can only modify the trigger type (with restrictions). The trigger source is fixed and set to receive a trigger through the rear-panel **PAT TRIG** connector. On the master, you can change both the trigger type (with restrictions) and the trigger source. The trigger source provides three options for triggering the waveforms: external trigger, front-panel **Trigger** key, or the GPIB trigger.

If the trigger settings are other than what the BBG synchronization feature supports, the feature changes the trigger settings to what is shown on [page 158](#). When this change occurs, the Agilent MXG generates a settings conflict error to alert you to the changes. To avoid the error generation,

appropriately configure the trigger settings prior to selecting a signal generator as the master or slave.


The system trigger propagates in the same manner as the synchronization pulse initiated by the master (see [System Synchronization](#)). So if it is not turned off during changes to the synchronization parameters, it can cause a false In Sync status.

The signal generator does not reset the trigger parameters when the multiple BBG synchronization feature is turned off. To play waveforms after disabling the feature, you must either set the trigger type to **Free Run** or provide a trigger to start the waveform play back.

Equipment Setup

Figure 8-18 Multiple Baseband Synchronization Setup

Note: To minimize synchronization delay, the Agilent BNC cable 10502A is the recommended cable for the rear-panel daisy chain connections (see [page 160](#)).

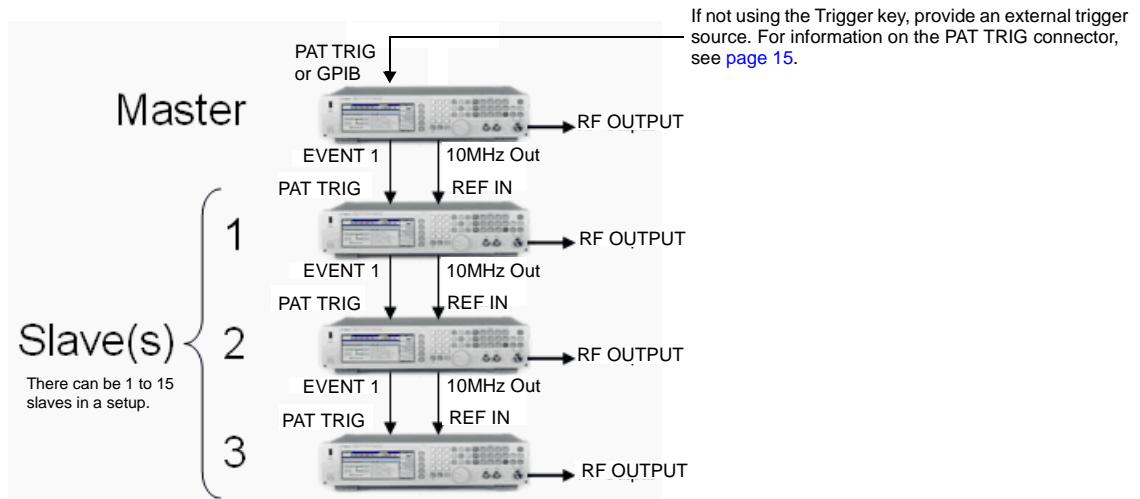

Configuring the Setup

Set the Common Parameters

Perform the following steps on all signal generators:

1. Set the frequency of the carrier signal.
2. Set the power level of the carrier signal.
3. Select the desired waveform (see [page 98](#)).

Do *not* turn the Dual ARB on.

4. Except for triggering, set the desired waveform parameters such as markers and sample clock.
The baseband synchronization feature limits the trigger selections for both the master and slaves. If the current trigger settings include unsupported BBG synchronization parameters, the Agilent MXG generates a settings conflict error and changes the trigger settings. To avoid the settings conflict error, manually set the trigger parameters as shown on [page 158](#) prior to setting the multiple BBG synchronization parameters.
5. Turn on the RF Output.

Set the BBG Synchronization Master Parameters

1. Press **Mode > Dual ARB > ARB Setup > More > Multi-BBG Sync Setup > Multi-Bbg Sync Type > Master**.
2. Set the number of slaves using the **Number of Slaves** softkey.
3. If desired, modify the trigger parameters (see [page 158](#)).
The master signal generator allows the modifications of both the trigger type and the trigger source.
 - a. Return to the Dual ARB menu (see [page 158](#)).
 - b. Set the desired trigger type and source.
 - c. Return to the **Multi-BBG Sync Setup** menu.

Set the BBG Synchronization Slave Parameters

1. Press **Mode > Dual ARB > ARB Setup > More > Multi-BBG Sync Setup > Multi-BBG Sync Type > Slave**.
2. Set the number of Slaves using the **Number of Slaves** softkey.
3. Set the slave position that the signal generator occupies.
There can be up to fifteen slaves in a system.
4. Press the **Listen for Sync** softkey and verify that Waiting for Sync appears in the Status area of the display.
5. If desired, select a different trigger type parameter:
 - a. Return to the Dual ARB menu (see [page 158](#)).
 - b. Set the desired trigger type.
 - c. Return to the **Multi-BBG Sync Setup** menu.
6. Repeat for each slave signal generator in the system.

Synchronize the System

Perform this procedure only after setting the parameters for both the master and slave signal generators. If resynchronizing a system, use the procedure “[Making Changes to the Multiple Sync Setup and Resynchronizing the Master/Slave System](#)” on page 163.

1. On the master, press the **Sync Slaves** softkey.

NOTE All of the signal generators in the master/slave system must be resynchronized when any changes are made to the master/slave settings or with the addition of a slave instrument, even if In Sync appears after pressing the **Listen for Sync** softkey on the slave instruments.

2. On the front panel displays, ensure that all of the signal generators show In Sync as the Status.

Trigger and Play the Waveform

1. On all Agilent MXGs, press **Mode > Dual ARB > ARB Off On** to On.
2. Start the trigger signal going to the master signal generator.

Making Changes to the Multiple Sync Setup and Resynchronizing the Master/Slave System

If any changes are made to the master/slave parameters or a signal generator (slave unit) is added to the system, the system must be resynchronized even if In Sync appears in the Status portion of the display.

1. Turn off the trigger source. If using the **Trigger** key, there is nothing to turn off.
If the trigger source is on and provides a continuous pulse stream, it may cause the signal generators to incorrectly display In Sync as the status after pressing the **Listen for Sync** softkey.
2. On each of the signal generators, press **Mode > Dual ARB > ARB Off On** to Off.
If a signal generator(s) has the Dual ARB on during changes, signal generators further in the chain may incorrectly display In Sync after pressing the **Listen for Sync** softkey.
3. On each of the signal generators, press **ARB Setup > More > Multi-BBG Sync Setup**.
4. Make the changes in the Multi-BBG Sync Setup menu.
Out Of Sync appears as the status message.
5. On each of the slave signal generators, press **Listen for Sync**.
6. Ensure that all of the slaves' Status show Waiting for Sync. If In Sync shows as the status, perform the following steps:
 - a. Check that the **PATT TRIG** to **EVENT 1** cables are properly connected on the rear-panel.
A disconnected cable can cause a false In Sync status.
 - b. If the cables are connected, perform steps 1 and 2.
 - c. Press **Listen for Sync** and ensure that Waiting for Sync appears as the status.
7. On the master signal generator, press **Sync Slaves**.
8. Verify that In Sync appears as the status on all master/slave signal generators.
9. Perform the process “[Trigger and Play the Waveform](#)” on page 163.

Waveform 5-Pack Licensing (Options 221-229)

Waveform 5-Pack licensing enables you to create, generate, and permanently license up to 45 Signal Studio waveforms (e.g. Each Option 22x enables licensing of five waveforms (Option 221, 222, 223, ... 229).

Each Waveform 5-Pack License includes one N7699A-D01 30-day Signal Studio demo license. N7699A-D01 allows access to all N76xxB Signal Studio software products to create and generate signals for 30 days so you can build, test, and license individual waveforms of your choice.

To redeem Option 22x and N7699A-D01, refer to the *N5182A-22x Entitlement Certificate* that comes with the N5182A-22x order.

Use the signal generator to manage the licensing of these waveforms. For example, you can use the signal generator to select individual waveforms for licensing and you can view a list of all currently licensed waveforms.

Understanding Waveform 5-Pack Licensing

Waveforms licensed with 5-Pack cannot be *exchanged*. Once a waveform is licensed, that license is permanent and cannot be revoked or replaced. Option 22x waveform licenses are signal generator specific (i.e. signal generator serial number specific).

Waveform 5-Pack licensing enables you to create and generate signals which can be saved for unlimited use in a signal generator (i.e. Waveform 5-Pack Option 22x is a *perpetual fixed* waveform license).

Use the Signal Studio software to build and download waveforms to the signal generator's volatile memory to be played. When you are satisfied with the waveform, it must be stored to non-volatile memory before it can be licensed.

If a licensed Option 22x waveform file is transferred to another signal generator, the file must be licensed by a separate Option 22x that is in the other signal generator *before* it can be played. For more information on extracting and downloading waveform files, refer to the *Programming Guide*.

To license additional waveforms that exceed the number permitted by an Option 22x, you must purchase an Option 22x that you do *not* already own. For example if you already own Option 221 with only two remaining licenses and you need ten more waveforms, purchase Options 222 and 223 to have enough licenses to license ten more waveforms. This would leave two remaining licenses on Option 223. (Repurchasing Option 221 a second time, for the *same* signal generator, gives you no additional Waveform 5-Pack licenses.)

Each Option 22x comes with a redeemable certificate for the N7699A-D01 30-day Signal Studio demo license. The 30-day countdown for N7699A-D01, begins at the time of the redemption. For maximum usage when purchasing multiple Option 22x, only redeem one N7699A-D01 at a time (e.g. after the first 30-day N7699A-D01 license expires, redeem the 2nd, etc.). This maximizes the time allowed for waveform creation using the N7699A-D01 30-day Signal Studio demo license (refer to the *N5182A-22x Entitlement Certificate*). N7699A-D01 30-day Signal Studio demo license *cannot* be purchased separately from Option 22x.

Downloaded waveforms can be licensed either during the N7699A-D01's 30 days or after the 30 days expire. However, after expiration of the N7699A-D01, you cannot playback any unlicensed downloaded waveform until it is licensed using the Waveform 5-Pack License Option 22x.

After licensing a waveform, you can make copies of the waveform using different file names for use on the same signal generator and even rename the original file without affecting the waveform license.

You can also use the Option 22x to license waveforms from N76xxB Signal Studio software downloaded during its 14-day free trial license. All of the N76xxB Signal Studio software products provide a 14-day trial period (trial license). This 14-day trial license lets you download and play back waveforms during the trial period. These waveforms are denoted by the TRL in the status message area of the waveform segment catalog. After the trial period expires, the TRL message is removed but the waveform remains. You can license these waveforms after the TRL message is gone.

Waveform 5-Pack requires firmware version \geq A.01.20.

Installing an Option N5182A-22x Waveform 5-Pack Licensing

1. Load a Waveform 5-Pack license, Option N5182A-22x, into the signal generator using License Manager or a USB media. For more information on loading the Waveform 5-Pack License, refer to the *N5182A-22x Entitlement Certificate*.
2. Redeem the N7699A-D01 that came with your copy of Option 22x. For more information on redeeming the N7699A-D01, refer to the *N5182A-22x Entitlement Certificate*.

Licensing a Signal Generator Waveform File

1. Create the waveform:
 - a. Download any of the N76xxB Signal Studio software that interest you. For downloading N76xxB Signal Studio software, refer to the N5182A-22x Entitlement Certificate.
 - b. Create and download a waveform to a signal generator using any of the N76xxB Signal Studio software. Refer to your *Signal Studio* software Help.

Waveform 5-Pack Licensing Softkeys Overview

Figure 8-19 Waveform 5-Pack licensing Softkeys

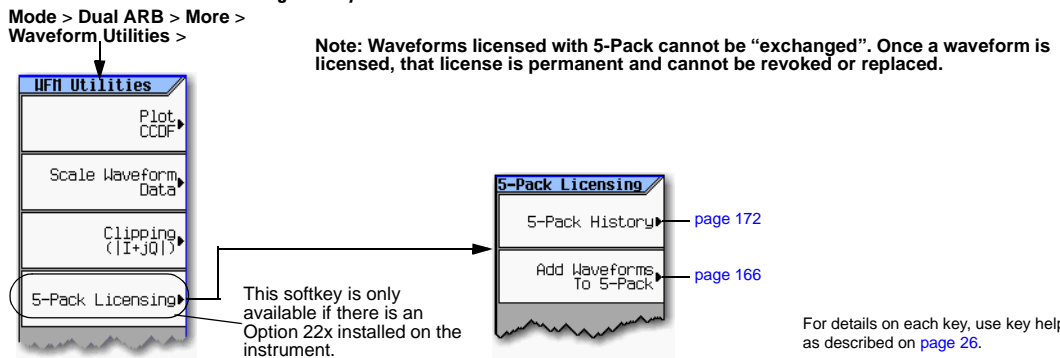


Figure 8-20 Add a Waveform to 5-Pack Softkeys

Mode > Dual ARB > More >
 Waveform Utilities > 5-Pack
 Licensing > Add Waveforms to
 5-Pack

Note: Waveforms licensed with 5-Pack cannot be “exchanged”. Once a waveform is licensed, that license is permanent and cannot be revoked or replaced.

This softkey is only active when there are secure waveforms that can be added and a Waveform 5-Pack license with available slots (i.e. if a waveform is already licensed or does not require licensing the softkey is greyed out). Refer to [page 170](#).

FREQUENCY	AMPLITUDE	Add To 5-Pack
2.412 000 000 00 GHz	-30.00 dBm	Add Waveform
I/Q ARB		
Catalog of Stored Segment Files in Int Storage Waveform Status		Catalog Type (Stored Segments)
Licenses Used: 1/45		
12TONE_WFM	5-Pack License Not Required	
AUTOGEN_WAVEFORM_XXX	5-Pack License Not Required	
CDMA2K_SCHAN_WFM	5-Pack License Not Required	
CDMA2K_PILOT_WFM	5-Pack License Not Required	
EDGE_BURST_WFM	5-Pack License Not Required	
GSM_BURST_WFM	5-Pack License Not Required	
N7602B_1	5-Pack Licensed	
N7602B_2		
N7615B_1	5-Pack License Not Required	
N7615B_2	5-Pack License Not Required	
10:16		

To select a waveform to receive one of your Waveform 5-Pack licenses, use the arrow keys to highlight the waveform and then press **Add Waveform**.

Displays the name of the Waveform file and status. Refer to [Table 8-3 on page 167](#).

This softkey displays a catalog of the waveform segments stored in the **Int Storage** or **USB Media**.

FREQUENCY	REF	AMPLITUDE	Catalog Type
935.200 000 00 MHz		-10.00 dBm	Stored Segments
Catalog of Stored Segment Files in Int Storage Waveform Status			BBG Segments
Licenses Used: 1/45			
12TONE_WFM		5-Pack License Not Required	
AUTOGEN_WAVEFORM_XXX		5-Pack License Not Required	
CDMA2K_SCHAN_WFM		5-Pack License Not Required	
CDMA2K_PILOT_WFM		5-Pack License Not Required	
EDGE_BURST_WFM		5-Pack License Not Required	
GSM_BURST_WFM		5-Pack License Not Required	
N7602B_1			
N7602B_2			
N7615B_1		5-Pack License Not Required	
N7615B_2		5-Pack License Not Required	
09:13			

This softkey displays a catalog of the waveforms stored in the **BBG** memory.

For details on each key, use key help as described on [page 26](#).

Table 8-3 Waveform 5-Pack Licensing Status Messages for the “Catalog of Segment Files in Int Storage [or USB Media]”

Status Message	Meaning	Notes
<i>Empty field</i>	If no status message, then the waveform is licensable.	<p>Once a Trial (TRL)^a license expires, the waveform becomes licensable (i.e. the status message for the TRL waveform becomes an <i>empty field</i>).</p> <p>If a licensed Option 22x waveform file is downloaded to <i>another</i> N5182A signal generator, the waveform becomes licensable on that <i>other</i> signal generator (i.e. the status message field is <i>empty</i>).</p>
5-Pack Licensed	This waveform is licensed by Option 22x.	
5-Pack License Not Required	<p>This status message applies to:</p> <p>Any free waveforms provided with the Agilent MXG (e.g. RAMP_TEST_WFM, and SINE_TEST_WFM, etc.)</p> <p>Any customer created waveform</p> <p>Any waveforms that have a valid license (e.g. Trial (TRL) licenses, Advanced Design System (ADS), etc.).</p>	<p>Once a Trial (TRL) license expires, the waveform becomes licensable (i.e. the status message for the TRL waveform becomes an <i>empty field</i>).</p> <p>If a licensed Option 22x waveform file is downloaded to <i>another</i> N5182A signal generator, the waveform becomes licensable on that <i>other</i> signal generator (i.e. the status message field is <i>empty</i>).</p>

^aTrial license (TRL) is *not* applicable to N7699A-D01. A license downloaded with N7699A-D01 *always* has an empty field before it is licensed with Option 22x. A Trial license is *not* licensable with Option 22x until *after* the 14-day trial expires.

Example: Licensing a Signal Studio Waveform


The following steps add a single waveform file, to a Waveform 5-Pack license. Refer to [Figure 8-22 on page 170](#).

2. There are two methods to save a waveform to the internal memory:

NOTE Before you can license a waveform with the Waveform 5-Pack licensing, the waveform must be saved in either the internal storage or the USB media.

- a. Save the file to internal storage using the **Backup Waveform To Int Storage** softkey:
 1. Press **Return > Return > More > Waveform Utilities > 5-Pack Licensing > Add Waveforms to 5-Pack**.
 2. Press **Backup Waveform To Int Storage** (refer to [Figure 8-21](#)).

Figure 8-21 Backup Waveform To Int Storage softkey

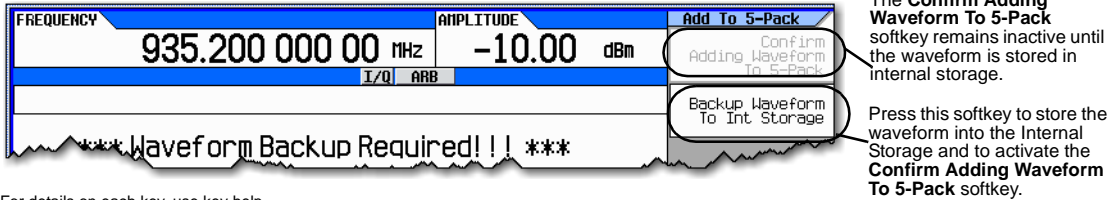

For details on each key, use key help as described on [page 26](#).

3. Go to [Step d](#).
- b. If the waveform has *already* been stored in the signal generator using the **Backup Waveform to Int Storage** softkey then proceed to [Step d](#).
 1. Otherwise use the ARB Segments menu Load **Store** softkey to store the waveform to internal storage. Refer to [“Working with Files” on page 45](#).
 2. Proceed to [Step 3](#) once you’ve stored the waveform to internal storage (internal media).
3. License the waveform:

- a. Press **Return > Return > More > Waveform Utilities > 5-Pack Licensing > Add Waveforms to 5-Pack**.

The signal generator displays a catalog of files labeled: Catalog of BBG Segment Files in BBG Memory.

- b. Use the arrow keys to highlight and select the file to be licensed.
- c. Press **Add Waveform**.

A warning is displayed: ***** Waveform Licensing Warning!!! *****. *If necessary, verify you have selected the correct waveform you want for licensing by pressing **Return***. Otherwise continue to the next step (refer to [Figure 8-22 on page 170](#)).

- d. Press **Confirm Adding Waveform to 5-Pack**.

The display returns to the Catalog of BBG Segment Files in BBG Memory and the file’s Status column is now labeled 5-Pack Licensed (refer to [Figure 8-22 on page 170](#)).

- e. Make a backup copy of this waveform on a USB media or a computer (*If the waveform is lost or deleted on the signal generator it cannot be recovered*).


CAUTION It is important that a *backup* copy is made of any 5-Pack waveforms; the backup copy must be stored on a computer or other media. *Do not store the backup copy on the signal generator. If all of the copies of the waveforms are deleted or lost, then there is no way to recover the waveform or reassign the license.* Refer to [“Working with Files”](#) on page 45.

Figure 8-22 Add Waveform to 5-Pack Softkey

Mode > Dual ARB > More >
 Waveform Utilities > 5-Pack
 Licensing > Add Waveforms to
 5-Pack



Status area for the waveform N7602B-WFM1 is empty and the **Add Waveform** softkey is active, indicating the waveform is licensable.

Important! Always backup licensed waveforms in a separate place from the instrument (e.g. computer, USB media, etc.).

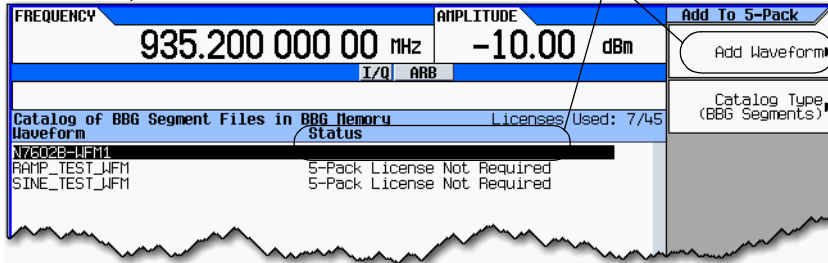

If the waveform selected for licensing has been verified as the waveform you want to be licensed, press **Confirm Adding Waveform To 5-Pack**.
Caution! This step cannot be undone.

This warning message indicates that this is the last chance for verifying that the waveform being licensed is the one you want. If the waveform selected has not been verified, press **Return** and verify the selection.

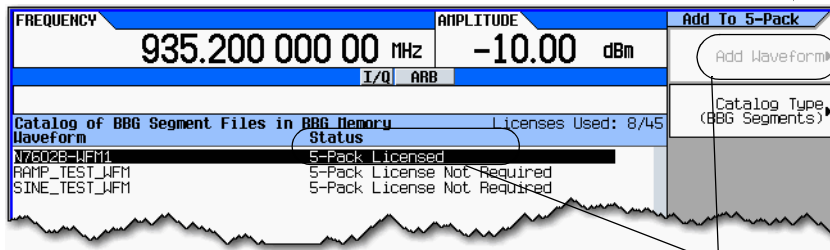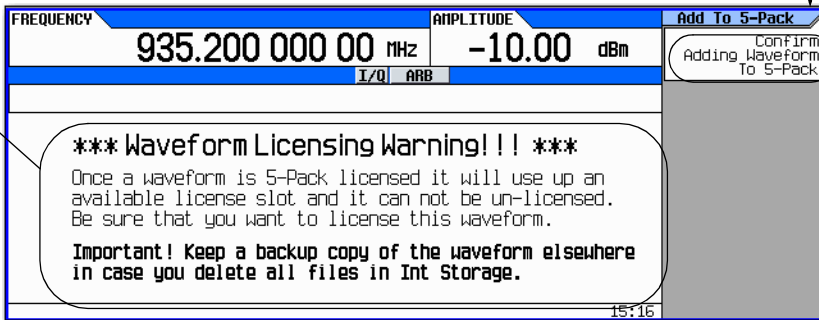

Note that N7602B-WFM1 has a Status of "5-Pack Licensed" and the **Add Waveform** softkey is no longer active.

For details on each key, use key help

Using Waveform 5-Pack History

The Waveform 5-Pack History softkeys can be used to manage the Waveform 5-Pack files on your signal generator. The 5-Pack History softkeys can be used to:

- Create a list for a specific Waveform 5-Pack licensed waveform including any *renamed* files that have been leveraged from that licensed waveform
- Create a list of all licensed and unlicensed waveforms on the signal generator

Refer to [Figure 8-23 on page 172](#), for a description of the Waveform 5-Pack History softkeys.

The **5-Pack History** softkey is only active, if you have *previously* stored a Waveform 5-Pack file in non-volatile memory (internal storage, or USB media). But, the softkey **5-Pack History** tracks the history of licensed waveform files that may no longer be available in non-volatile memory (e.g. if the waveform file has been deleted from internal storage or is located on a USB media that is *not* attached to the instrument, *the 5-Pack History softkey remains active*). 5-Pack History retains a catalog of the Redemption Date, Waveform ID, and the Original Filename.

NOTE You can display either a catalog of the Internal storage or of the USB media but *not* both at the same time.

If you switch from the internal storage to the USB media, and the instrument displays an “Error -230, Data corrupt or stale” this is typically because a file (or files) was found with the same name, but the file is a *different waveform file* (has a *different* Waveform ID) than the original 5-Pack licensed internal storage file.

Figure 8-23 Waveform 5-Pack History Softkeys

Mode > Dual ARB > More >
Waveform Utilities > 5-Pack
Licensing > 5-Pack History

Only available when there have been waveforms with Waveform 5-Pack licenses previously stored.

Pressing this softkey searches for every copy of the highlighted waveform regardless of the current filename. If the search returns no results, then the original waveform has been deleted and cannot be found.

Waveform 5-Pack License History	Redemption Date	License History	Waveform ID	Original Filename
	05/03/2007	df344ee3		N7602B_1
	05/03/2007	df362ee3		N7602B_2
	05/03/2007	df374ee3		N7602B_3

Licenses Used: 3/45

This area displays the date the waveform was licensed, the unique Waveform ID, and Original filename at the time the waveform was first redeemed.

This screen displays all waveforms that are licensed by Option 22x.

For details on each key, use key help as described on page 26.

Location	Current Filename	All Waveforms
Int Storage	N7602B_1_COPY1	
Int Storage	N7602B_1_COPY2	
Int Storage	N7602B_1_COPY3	
Int Storage	N7602B_2	
Int Storage	N7602B_3	
BBG Memory	N7602B_1_COPY3	

Location is the memory location:

*Int Storage
*BBG Memory, Or
*USB Media

Note:

- 1) In this example, the waveform N7602B_1_COPY3 is stored in the Int Storage and playing in the BBG Memory.
- 2) In this example, the Int Storage has been selected as the non-volatile storage location. To view any 5-Pack waveforms stored on the USB media, the USB media must be selected as the default storage. Refer to page 45.

When you press Find Waveform, any copies of the originally saved waveform are displayed on the instrument (e.g. N7602B_1_COPY1, N7602B_1_COPY2, and N7602B_1_COPY3). In this example, the original filename N7602B_1 was not found because the original file was deleted or the name was changed. But three copies were found (N7602B_1_COPY3 was found in both the Int Storage and the BBG Memory).

Location	Current Filename	All Waveforms
Int Storage	N7602B_1_COPY1	N7602B_1
Int Storage	N7602B_1_COPY2	N7602B_1
Int Storage	N7602B_1_COPY3	N7602B_1
BBG Memory	N7602B_1_COPY3	N7602B_1

Example: Finding the History of a Waveform 5-Pack License

Use the following procedure to create a catalog of licensed Waveform 5-Pack files in the internal storage or USB media. Refer to [Figure 8-24 on page 173](#), for the following procedure.

The following procedure generates a catalog for a Waveform 5-Pack file labeled: N7602B-WFM1.

1. On the signal generator:
 - a. Press **Mode > Dual ARB > More > Waveform Utilities > 5-Pack Licensing > 5-Pack History**
 - b. Use the arrow keys to highlight the cataloged file N7602B-WFM1.
 - c. Press **Find Waveform**

The instrument displays a catalog titled “Waveform 5-Pack Search Results”. This catalog displays a list of all of the files that are copies of the original file that was licensed with the Waveform 5-Pack licensing, named N7602B-WFM1. For this example, the copies are currently in the BBG memory and the Internal storage and named N7602B-WFM1 and N7602B-WFM1_COPY (respectively). Refer to [Figure 8-24 on page 173](#).

NOTE If no files are found, you can reload the backup copies that were made in [Step e on page 169](#).

Figure 8-24 Using Waveform 5-Pack History “Find Waveform” Softkey

Mode > Dual ARB > More > Waveform Utilities > 5-Pack Licensing > 5-Pack History

The highlighted file N7602B-WFM1 is the waveform created in this example. (Notice the unique Waveform ID displayed for each licensed waveform.)

For details on each key, use key help as described on [page 26](#).

FREQUENCY	AMPLITUDE	5-Pack History																											
6.000 000 000 00 GHz	-144.00 dBm	Find Waveform																											
		Find All Waveforms																											
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 20%;">Waveform 5-Pack Redemption Date</th> <th style="width: 20%;">License History Waveform ID</th> <th style="width: 60%;">Original Filename</th> </tr> </thead> <tbody> <tr> <td>05/03/2007</td> <td>df344ee3</td> <td>N7602B_1</td> </tr> <tr> <td>05/03/2007</td> <td>2c15a2ca</td> <td>N7602B_2</td> </tr> <tr> <td>05/10/2007</td> <td>fa45bc1c</td> <td>UNTITLED-WFM1</td> </tr> <tr> <td>05/10/2007</td> <td>42906a2e</td> <td>UNTITLED-WFM1</td> </tr> <tr> <td>05/10/2007</td> <td>0f8037d0</td> <td>UNTITLED-WFM1</td> </tr> <tr> <td>05/14/2007</td> <td>2fee68b2</td> <td>UNTITLED-WFM1</td> </tr> <tr> <td>05/16/2007</td> <td>b176a7da</td> <td>N7602B-WFM1</td> </tr> <tr> <td>05/16/2007</td> <td>bb240b05</td> <td>N7602B-WFM1</td> </tr> </tbody> </table>		Waveform 5-Pack Redemption Date	License History Waveform ID	Original Filename	05/03/2007	df344ee3	N7602B_1	05/03/2007	2c15a2ca	N7602B_2	05/10/2007	fa45bc1c	UNTITLED-WFM1	05/10/2007	42906a2e	UNTITLED-WFM1	05/10/2007	0f8037d0	UNTITLED-WFM1	05/14/2007	2fee68b2	UNTITLED-WFM1	05/16/2007	b176a7da	N7602B-WFM1	05/16/2007	bb240b05	N7602B-WFM1	<p>Licenses Used: 8/45</p>
Waveform 5-Pack Redemption Date	License History Waveform ID	Original Filename																											
05/03/2007	df344ee3	N7602B_1																											
05/03/2007	2c15a2ca	N7602B_2																											
05/10/2007	fa45bc1c	UNTITLED-WFM1																											
05/10/2007	42906a2e	UNTITLED-WFM1																											
05/10/2007	0f8037d0	UNTITLED-WFM1																											
05/14/2007	2fee68b2	UNTITLED-WFM1																											
05/16/2007	b176a7da	N7602B-WFM1																											
05/16/2007	bb240b05	N7602B-WFM1																											

— see [page 174](#).

FREQUENCY	AMPLITUDE	Find Waveform						
6.000 000 000 00 GHz	-144.00 dBm							
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 50%;">Waveform 5-Pack Search Results Location</th> <th style="width: 50%;">Current Filename</th> </tr> </thead> <tbody> <tr> <td>Int. Storage</td> <td>N7602B-WFM1_COPY</td> </tr> <tr> <td>BBG Memory</td> <td>N7602B-WFM1_COPY</td> </tr> </tbody> </table>		Waveform 5-Pack Search Results Location	Current Filename	Int. Storage	N7602B-WFM1_COPY	BBG Memory	N7602B-WFM1_COPY	N7602B-WFM1
Waveform 5-Pack Search Results Location	Current Filename							
Int. Storage	N7602B-WFM1_COPY							
BBG Memory	N7602B-WFM1_COPY							

Notice that the originally 5-Pack licensed waveform, N7602B-WFM1, has been changed to N7602B-WFM1_COPY and is saved in the Internal Storage and playing in the BBG Memory.

If no waveforms are listed when **Find Waveform** is pressed, then the waveform cannot be found in BBG Memory, Internal Storage, or USB Media.

Finding All Waveforms Associated with 5-Pack Licenses

The following procedure displays a catalog of *all* of the Waveform 5-Pack files in the BBG memory and the internal storage:


1. On the signal generator:
 - a. Press **Mode > Dual ARB > More > Waveform Utilities > 5-Pack Licensing > Find All Waveforms**

The instrument displays a catalog titled: Waveform 5-Pack Search Results. Refer to [Figure 8-25](#).

NOTE If no files are found, you can reload the backup copies that were made in [Step e](#) on [page 169](#).

Figure 8-25 Using Waveform 5-Pack History “Find All Waveforms” Softkey

**Mode > Dual ARB > More > Waveform Utilities >
 5-Pack Licensing > 5-Pack History > Find All
 Waveforms**

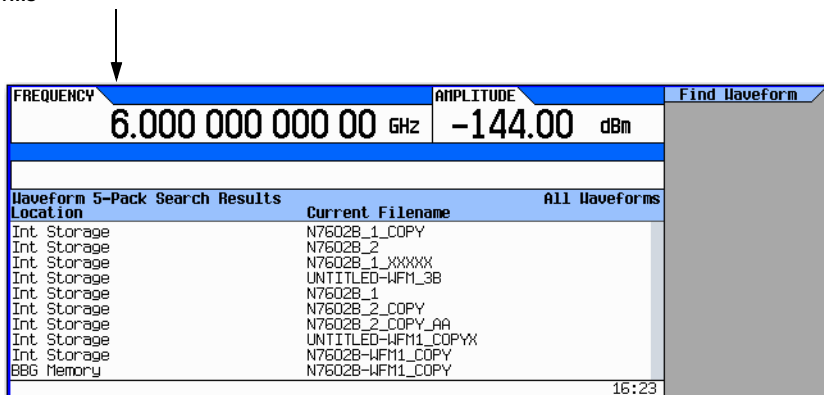

Waveform 5-Pack Warning Messages

Figure 8-26

The figure displays four sequential screenshots of the Agilent MXG signal generator's waveform licensing interface. Each screenshot shows the current frequency and amplitude settings, along with a 'Add To 5-Pack' button. The interface also displays various warning messages related to licensing, such as 'Waveform Licensing Warning', 'Waveform Backup Required', 'Waveform Backup Failed', and 'Waveform Renaming Required'. Arrows from the explanatory text on the right point to these specific warning messages.

Warning 1: Waveform Licensing Warning

*** Waveform Licensing Warning !!! ***
Once a waveform is 5-Pack licensed it will use up an available license slot and it can not be un-licensed. Be sure that you want to license this waveform.
Important! Keep a backup copy of the waveform elsewhere in case you delete all files in Int Storage.

Warning 2: Waveform Backup Required

*** Waveform Backup Required !!! ***
Waveform backup required. The waveform can not be licensed until it is copied to non-volatile memory.
You must back up the waveform to non-volatile memory before you can license it.

Warning 3: Waveform Backup Failed

*** Waveform Backup Failed !!! ***
Waveform backup failed. The waveform could not be copied to non-volatile memory. There may not be enough free memory.
You must free enough non-volatile memory to copy the waveform before you can license it.

Warning 4: Waveform Renaming Required

*** Waveform Renaming Required !!! ***
The file you are trying to license is not backed up in non-volatile memory, but a file in non-volatile memory has the same name.
You must rename one of the files before adding the waveform to the 5-Pack license list.

Explanatory Text:

- This standard warning is displayed every time a waveform is selected to be licensed. This notification indicates that one of the available "license slot[s]" is about to be used from Option 22x. **ALWAYS make backup copies of waveforms in a separate non-volatile memory in case a file is deleted or lost from the instrument's internal storage.**
- This warning is displayed when an attempt is made to license a waveform that has *not* been saved to internal storage or USB media (i.e. waveforms cannot be licensed unless they have been stored to non-volatile memory). Press the **Backup Waveform To Int Storage** softkey.
- This warning is displayed when there is insufficient memory or other problems with the internal storage, or USB media (non-volatile memory) and the waveform could not be saved to non-volatile memory.
- This warning is displayed when the file being licensed is *not* backed up in internal storage or the USB media (non-volatile memory), but there is a file *already* in the internal storage or USB media, with the same name.

Basic Digital Operation (Option 651/652/654)
Waveform 5-Pack Licensing (Options 221-229)

9 Adding Real Time Noise to a Signal (Option 403)

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting the power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

This feature is available only in N5182A Agilent MXG Vector Signal Generators with Option 431. Option 431 requires Option 651, 652, or 654.

This chapter contains examples of using the additive white gaussian noise (AWGN) waveform generator, which is available only in vector signal generators with Option 403.

- [“Adding Real-Time Noise to a Dual ARB Waveform” on page 178](#)
- [“Using Real Time I/Q Baseband AWGN” on page 181](#)

Adding Real-Time Noise to a Dual ARB Waveform

NOTE The procedures in this section that pertain specifically to adding Real-Time Noise (AWGN) to a waveform, are applicable to the Custom ARB, Multitone, and Two-Tone modulation standards too.

A vector signal generator with option 403 enables you to apply additive white gaussian noise (AWGN) to a carrier in real time while the modulating waveform plays in the dual ARB waveform player. This feature appears in each of the arb formats and as a stand-alone menu (Refer to [Figure 9-3 on page 181](#)).

Figure 9-1 Real Time I/Q Baseband AWGN Softkeys


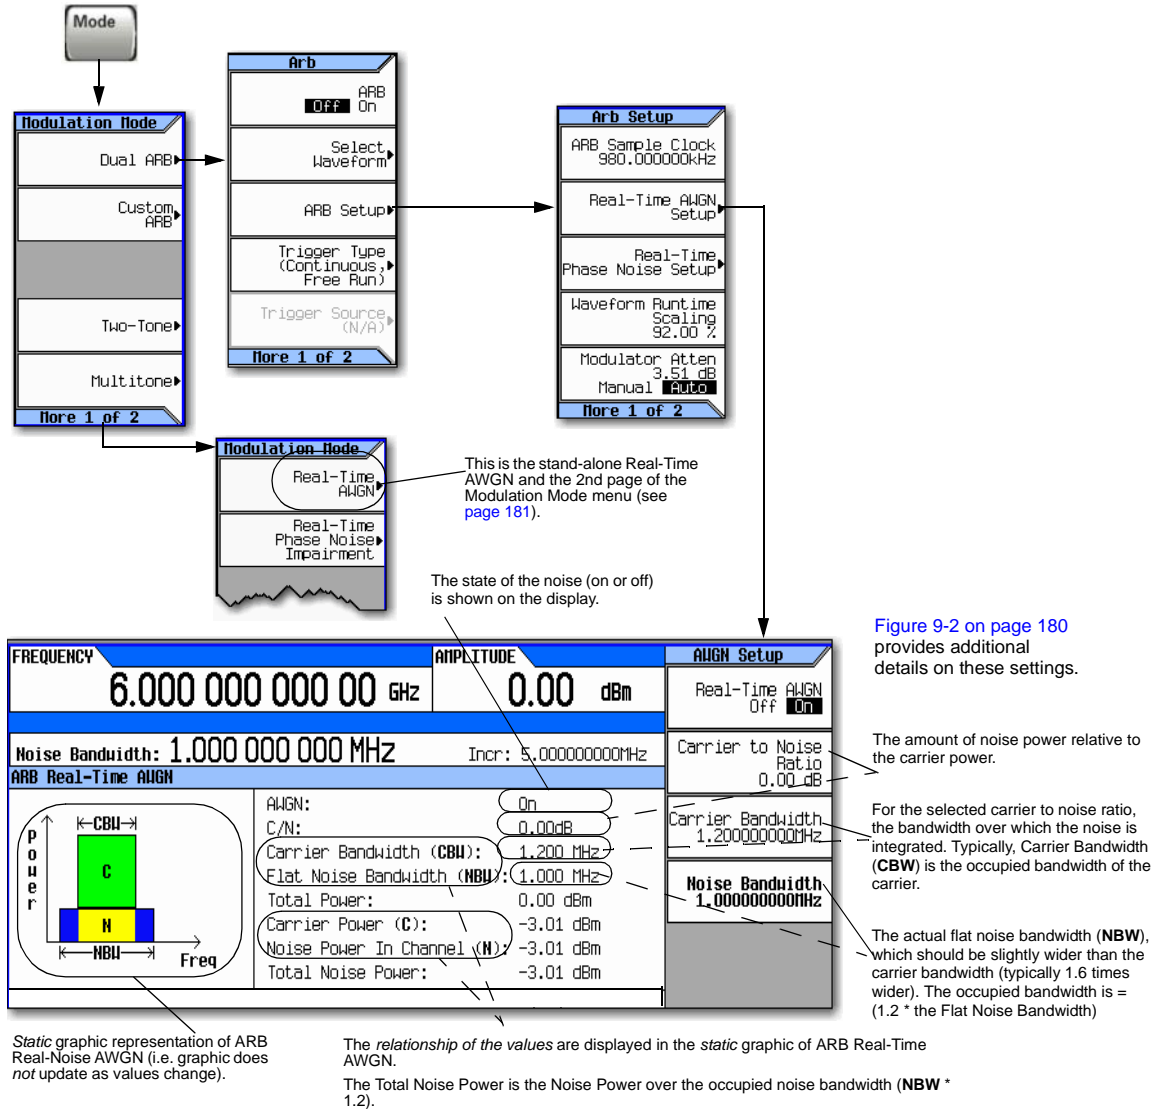


Figure 9-2 Carrier to Noise Ration Components

Carrier Bandwidth (CBW) is typically the occupied bandwidth of the carrier and the **Noise Bandwidth** is the *flat* noise bandwidth (NBW).

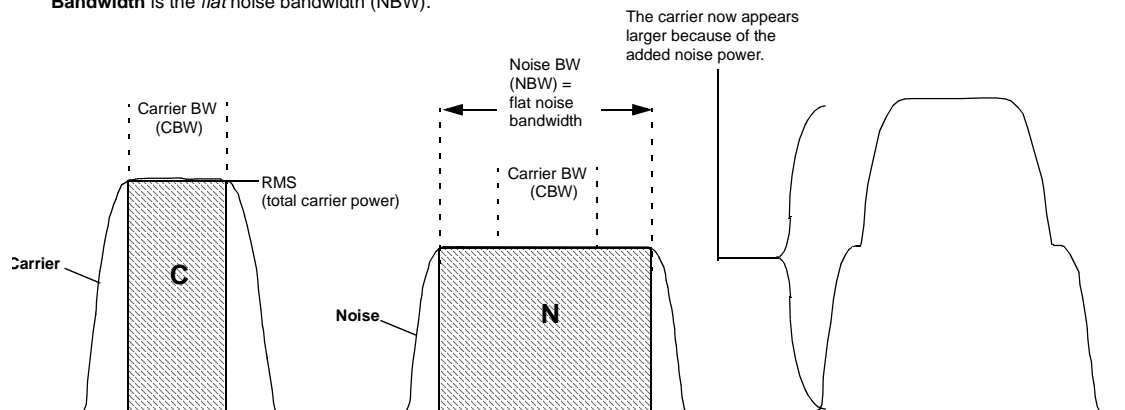

Example


Use the following steps to modulate a 1 GHz, -10 dBm carrier with the factory-supplied waveform SINE_TEST_WFM, and then apply noise with a 45 MHz bandwidth signal that has a 30 dB carrier-to-noise ratio across a 40 MHz carrier bandwidth.

1. Preset the signal generator and set the following:
 - Frequency: 1 GHz
 - Amplitude: -10 dBm
 - RF output: on
2. Select the factory-supplied waveform SINE_TEST_WFM:
 - a. Press **Mode > Dual ARB > Select Waveform**.
 - b. Highlight SINE_TEST_WFM and press **Select Waveform**.
3. Turn on the dual ARB player: press **ARB Off On** to highlight On.
4. Set the ARB sample clock to 50 MHz: Press **ARB Setup > ARB Sample Clock > 50 > MHz**.
5. Press **Real-time Noise Setup** and set the following:
 - Carrier to Noise Ratio: 30 dB
 - Carrier Bandwidth: 40 MHz
 - Noise Bandwidth: 45 MHz
 - Real-time Noise: on

The signal generator's displayed power level (-10 dBm) *includes* the noise power.

Using Real Time I/Q Baseband AWGN

Figure 9-3 Real Time I/Q Baseband AWGN Softkeys

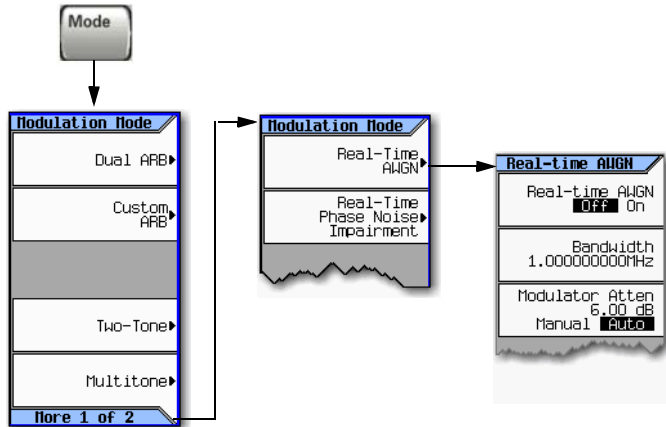

For details on each key, use key help as described on [page 26](#).


Use the following steps to apply 10 MHz bandwidth noise to a 500 MHz, -10 dBm carrier.

1. Configure the noise:
 - a. Preset the signal generator.
 - b. Press **Mode** > **Real Time I/Q Baseband AWGN**
 - c. Press **Bandwidth** > **10** > **MHz**.

2. Generate the noise:

Press **AWGN Off On** until **On** highlights.

During generation, the **AWGN** and **I/Q** annunciators activate (as shown at right). **AWGN** is now available to modulate the RF carrier.

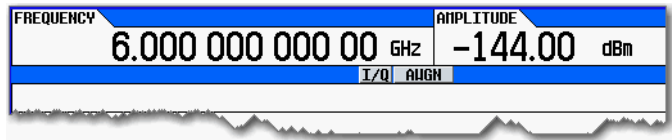

3. Configure the RF output:

- Frequency: 500 MHz
- Amplitude: -10 dBm
- RF output: on

The carrier with AWGN is now available at the signal generator's RF OUTPUT connector.

Adding Real Time Noise to a Signal (Option 403)
Using Real Time I/Q Baseband AWGN

10 Real-Time Phase Noise Impairments (Option 432)

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting the power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

This feature is available only in N5182A Agilent MXG Vector Signal Generators with Option 431. Option 431 requires Option 651, 652, or 654.


This chapter contains the softkey maps to locate the Phase Noise Impairment option functions and information on the use of this feature.

- [Real-Time Phase Noise Impairment](#) on page 184
- [The Agilent MXG Phase Noise Shape and Additive Phase Noise Impairments](#) on page 185
- [Understanding the Phase Noise Adjustments](#) on page 187
- [DAC Over-Range Conditions and Scaling](#) on page 188

Real-Time Phase Noise Impairment

This feature lets you degrade the phase noise performance of the signal generator by controlling two frequency points and an amplitude value. The signal generator adds this phase noise to the phase noise normally produced by the Agilent MXG. This feature appears in each of the arb formats and as a stand-alone menu. While the following figure shows how to access the controls using both the stand-alone menu and the Dual ARB player, the location and softkeys within each arb format is the same as for the Dual ARB player.

Figure 10-1 Stand-Alone and Dual ARB Player Real-Time Phase Noise Softkeys

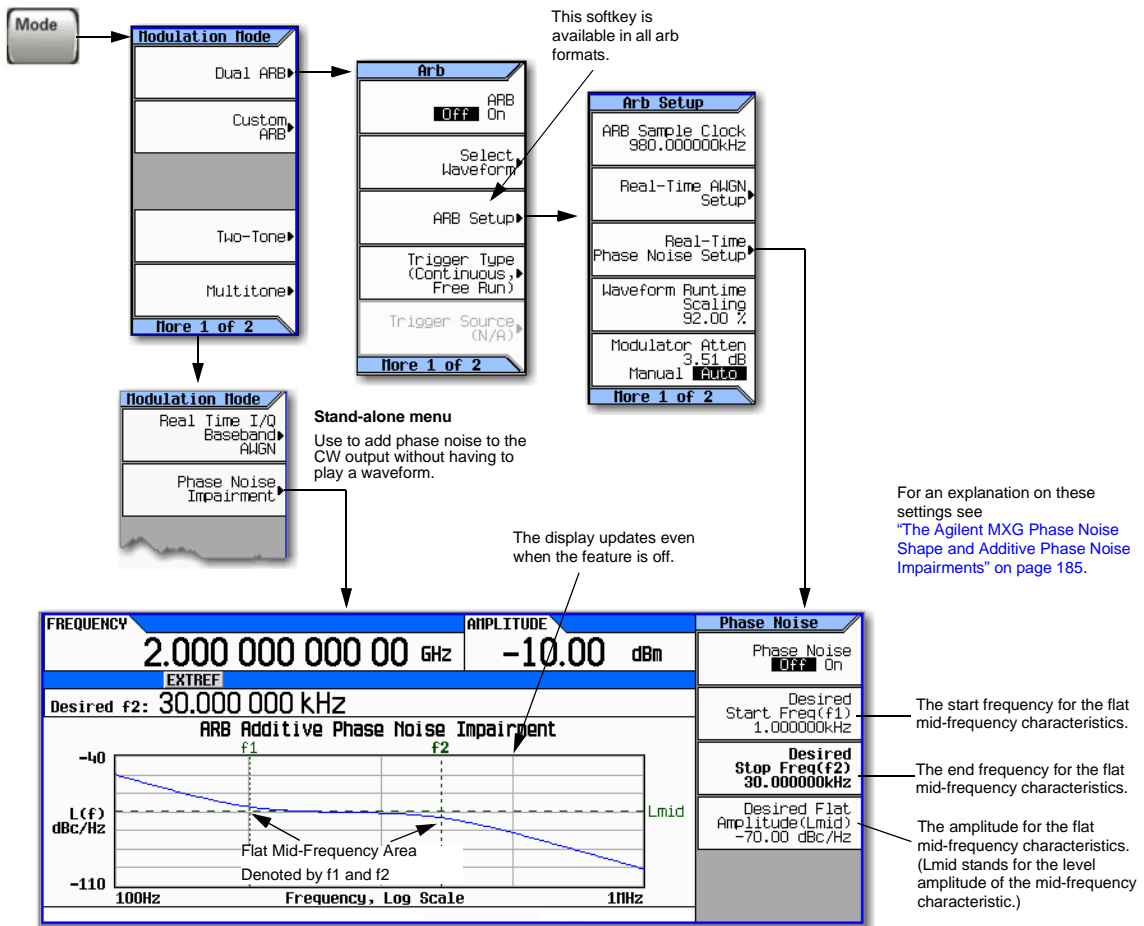


NOTE: The phase noise impairment is added to the base phase noise of the signal generator.

For details on each key, use key help as described on page 26.

The Agilent MXG Phase Noise Shape and Additive Phase Noise Impairments

Phase Noise Plots Without Phase Noise Impairment

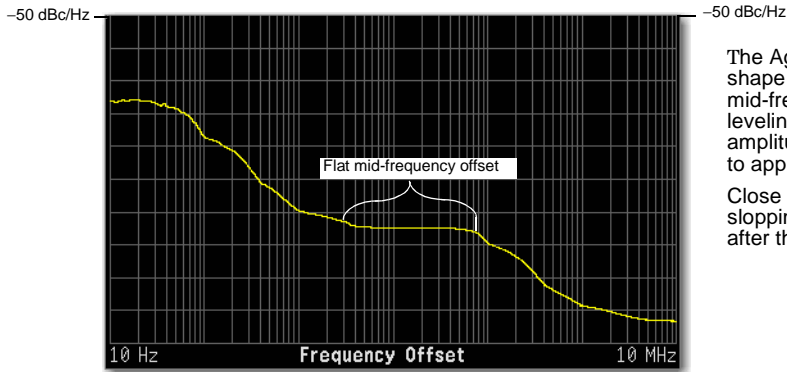


The Agilent MXG demonstrates a definitive shape to its phase noise plot. The mid-frequency offsets are characterized by a leveling (flattening) of the phase noise amplitude from approximately a 3 kHz offset to approximately a 70 kHz offset.

Close in and far out offsets demonstrate sloping characteristics (areas before and after the mid-frequency offsets).


The signal generator degrades the phase noise by moving the mid-frequency characteristics and/or changing its amplitude using the following settings:

- Start frequency (f_1) of the mid-frequency characteristics
- Stop frequency (f_2) of the mid-frequency characteristics
- Amplitude (L_{mid}) of the mid-frequency characteristics

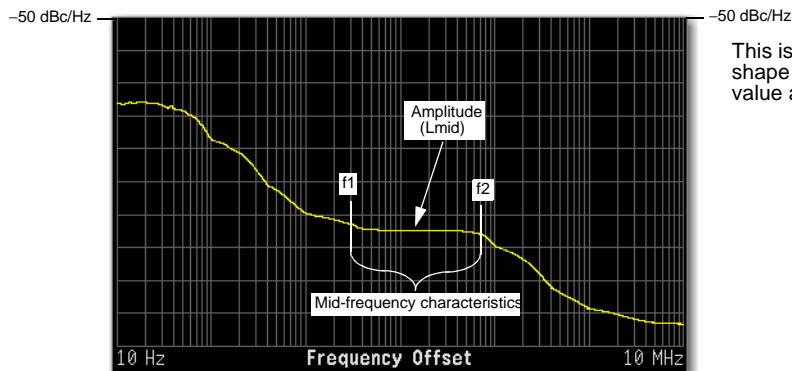


This is a plot of the unmodified phase noise shape that shows the location that each value alters.

Phase Noise Plots With Phase Noise Impairments

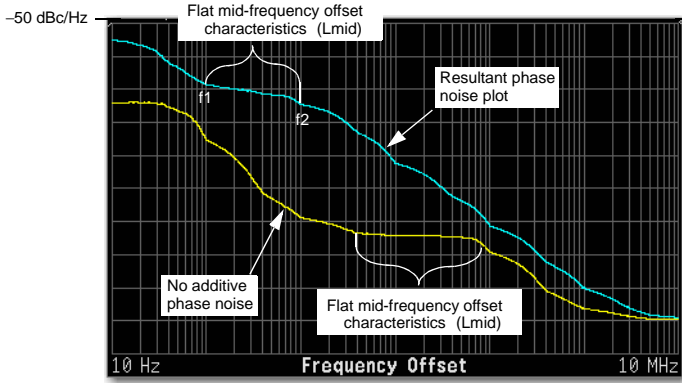

When turned on, this phase noise is added to the base phase noise of the signal generator.

Even though it is only the mid-frequency characteristics placement that are modified, these changes affect the entire phase noise shape. The close in and far out offset characteristics change by exhibiting approximately a 20 dBc/Hz slope for each octave of frequency offset.

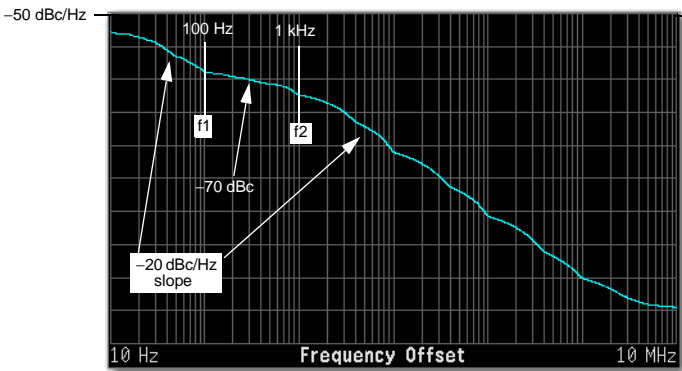


The resultant phase noise plot shown on the left has the following settings:

- $f_1 = 100 \text{ Hz}$
- $f_2 = 1 \text{ kHz}$
- Amplitude (L_{mid}) = -70 dBc

Ensure that the f_1 value is less than or equal to f_2 . If not, f_2 changes its value to match f_1 . Conversely if f_2 is set to a value that is less than f_1 , f_1 changes its value to match f_2 .

The frequency values entered for the impairments may not be the exact values when viewed on the RF output. The entered values are guidelines that the signal generator uses to calculate the real values. See “Understanding the Phase Noise Adjustments” on page 187 for more information.

To view the results of the settings (f_1 , f_2 , and L_{mid}), use the front panel graph (below and on page 184) or view the phase noise plot on a measurement instrument (shown above—Agilent E4440A PSA with Option 226).

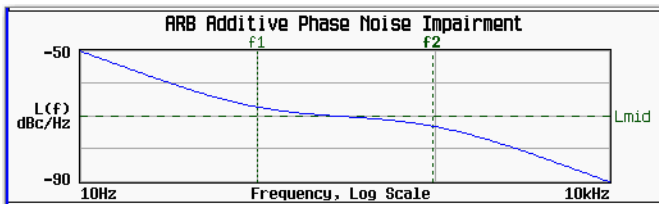

Signal generator front panel plot:

- $f_1 = 100 \text{ Hz}$
- $f_2 = 1 \text{ kHz}$
- $L_{mid} = -70 \text{ dBc}$

Understanding the Phase Noise Adjustments


The signal generator bases the resultant phase noise shape on three settings, Lmid (amplitude), f1 (start frequency), and f2 (stop frequency).

The range for Lmid is coupled to f2, so as f2 increases in value, Lmid's upper boundary decreases. If the current Lmid setting is too high for the new f2 setting, the signal generator changes the Lmid value and generates an error to alert you to the change. In addition, the actual Lmid value can vary by 0.28 dBc/Hz from the entered value.

The frequency settings (f1 and f2) are really guidelines that the signal generator uses to calculate the real frequency offset values seen on the RF OUTPUT. This means that the entered start and stop frequency values are an approximation and may not be the values seen on a measurement instrument, however they will be close.

The effects of the f1 and f2 parameters are based on a varying logarithmic scale. This scale is determined by the f2 value. The higher the f2 value the larger the scale, which makes this behavior more noticeable at higher frequency settings. This becomes apparent when a change in the f1 or f2 value causes little to no change in the f1 or f2 position. This is easy to view using the signal generator's front panel phase noise graph and demonstrated in Figure 10-2. This behavior makes the frequency adjustments coarser as the f2 frequency value increases.

Figure 10-2 f1 and f2 Frequency Setting Behavior

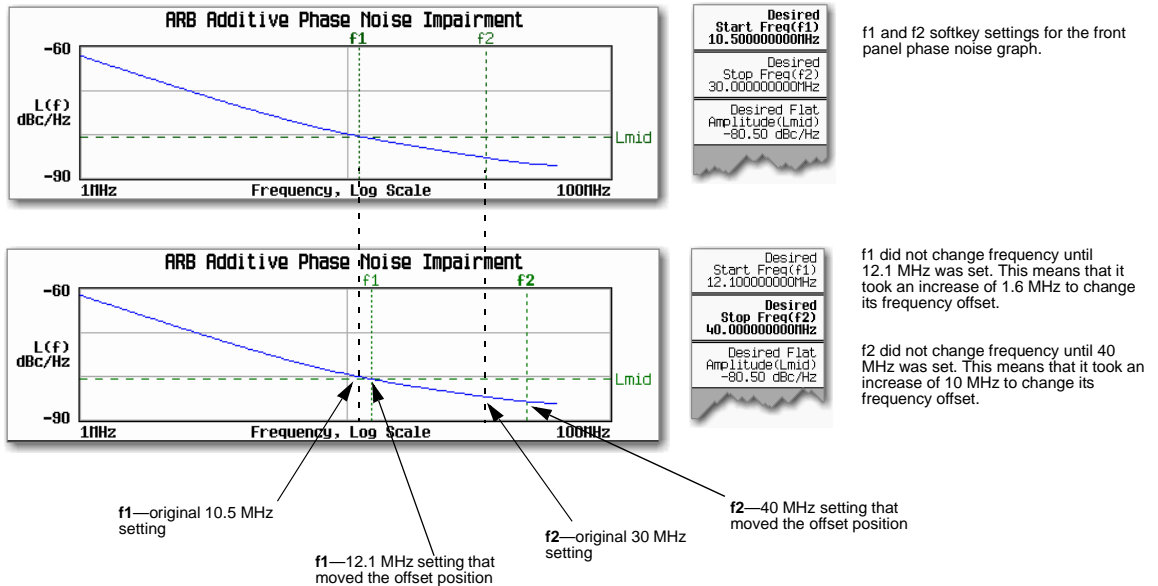

For details on each key, use key help as described on page 26.


The only way to make an accurate determination of the effect of the f1 and f2 values is by viewing the front panel graph or making a measurement. You can view the front panel graph remotely by using the LXI interface. For more information on the LXI interface, see the *Programming Guide*.

DAC Over-Range Conditions and Scaling

When using phase noise impairment, it is possible to create a DAC over-range condition, which causes the Agilent MXG to generate an error. To minimize this condition with the phase noise impairment feature, the Agilent MXG incorporates an automatic DAC over-range protection feature that scales down the I/Q data. Because it can scale the data by more than what is actually need, it typically decreases the dynamic range of the waveform. This is especially noticeable when using a constant amplitude signal such as GSM.

For the Dual ARB Player, the automatic over-range protection can be turned off (on is the factory default). The control for the Dual ARB DAC over-range protection feature is located in the key path as shown in [Figure 10-3](#).

Figure 10-3 Dual ARB DAC Over-Range Protection Softkey Location

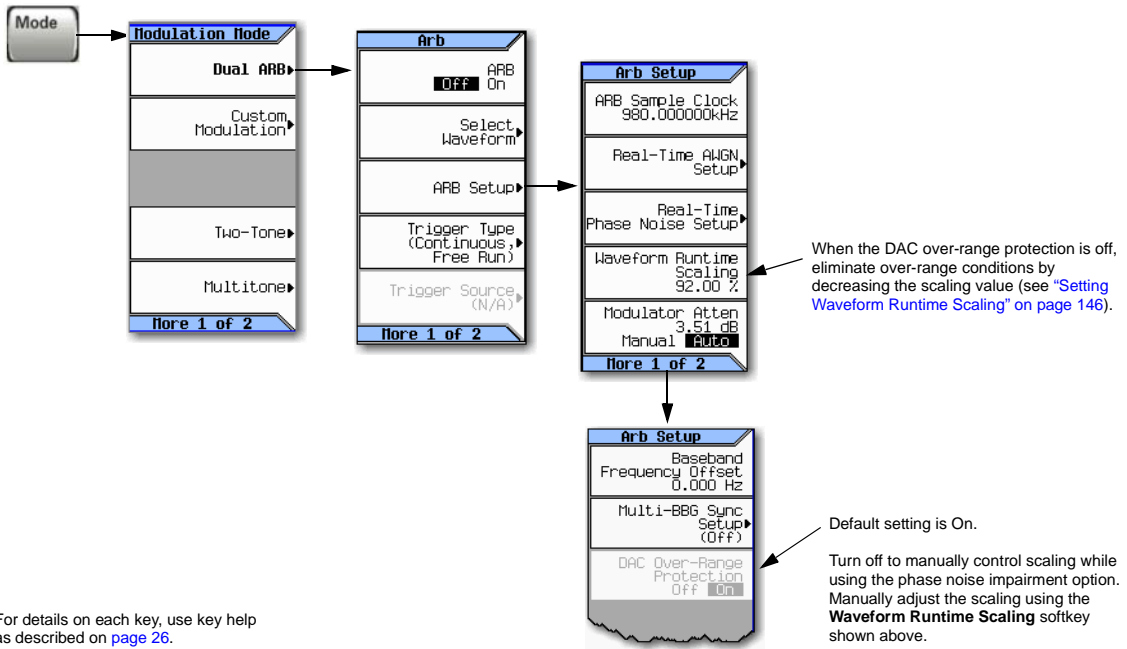

In the Dual ARB Player, to avoid excessive scaling or to just perform scaling manually, turn the over-range protection off and use the **Waveform Runtime Scaling** softkey to eliminate DAC over-range conditions.

When the automatic feature is disabled, the other options to eliminate a DAC over-range condition are to reduce the f2 value, or the Lmid value, or both until the condition corrects itself.

11 Custom Digital Modulation (Option 431)

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting the power level and frequency, refer to [Chapter 3, “Basic Operation,” on page 25](#) and familiarize yourself with the information in that chapter.

This feature is available only in N5182A Agilent MXG Vector Signal Generators with Option 431. Option 431 requires Option 651, 652, or 654.

- [Custom Modulation](#) on page 190
- [Using the Arbitrary Waveform Generator](#) on page 195
- [Using Finite Impulse Response \(FIR\) Filters](#) on page 204
- [Modifying a FIR Filter Using the FIR Table Editor](#) on page 208

Custom Modulation

Custom Modulation has built-in modulation standards such as TETRA and DECT; and pre-defined modulation types such as BPSK and 16QAM that can be used to create a signal in addition, it provides the flexibility to modify the digital format's attributes.

Custom Arb Waveform Generator

The signal generator's Arb Waveform Generator mode is designed for out-of-channel test applications. This mode can be used to generate data formats that simulate random communication traffic and can be used as a stimulus for component testing. Other capabilities of the Arb Waveform Generator mode include:

- configuring single or multicarrier signals. Up to 100 carriers can be configured.
- creating waveform files using the signal generator's front panel interface.

The waveform files, when created as random data, can be used as a stimulus for component testing where device performance such as adjacent channel power (ACP) can be measured. The AUTOGEN_WAVEFORM file, that is automatically created when you turn the Arb Waveform Generator on, can be renamed and stored in the signal generator's non-volatile memory. This file can later be loaded into volatile memory and played using the dual ARB waveform player.

For more information, refer to [Waveform File Basics](#) on page 96 and [Modes of Operation](#) on page 3.

Figure 11-1 Custom ARB Softkeys

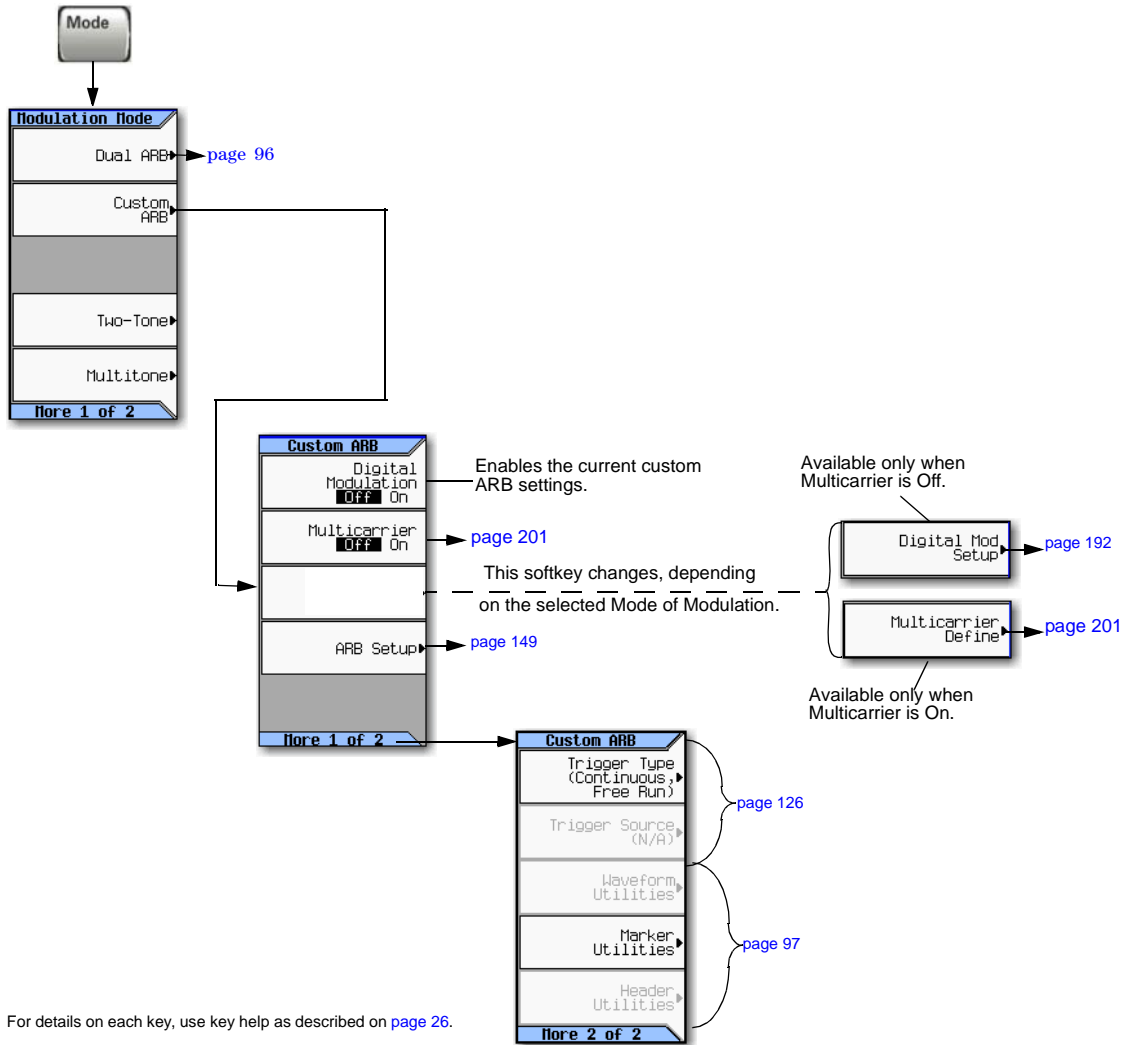


Figure 11-2 Quick Setup Softkeys

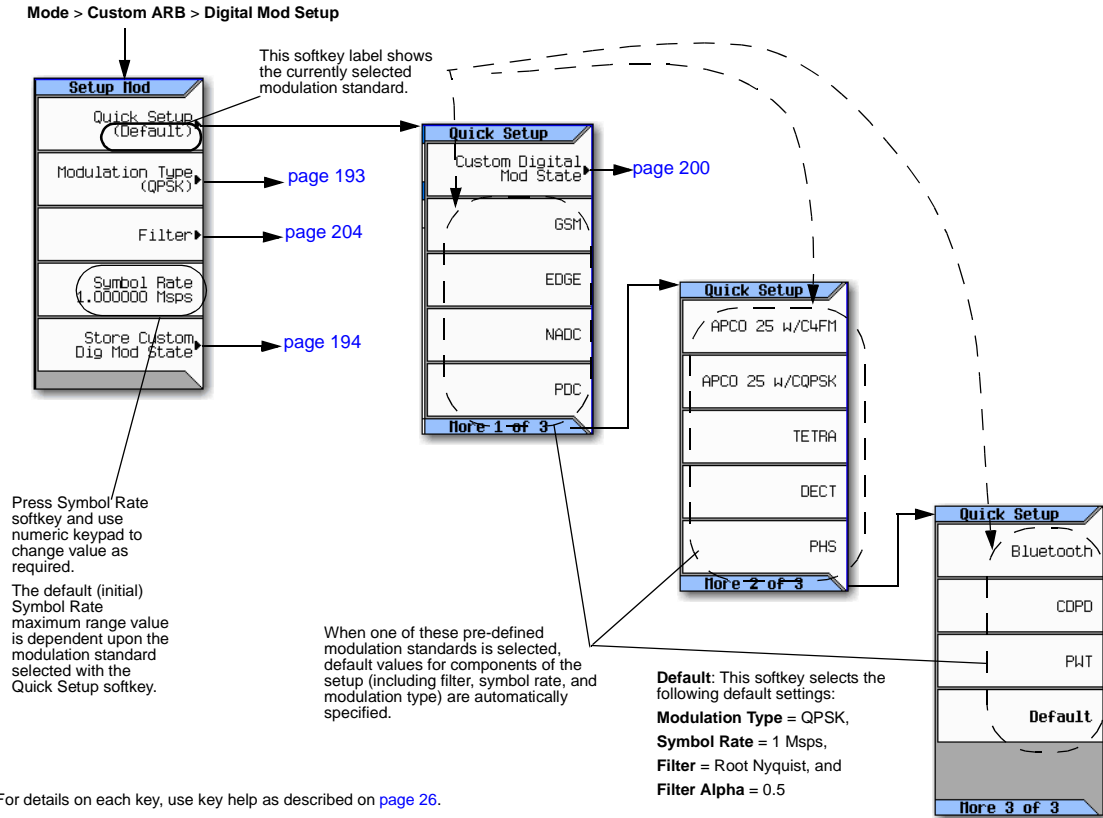


Figure 11-3 Mod Type Softkeys

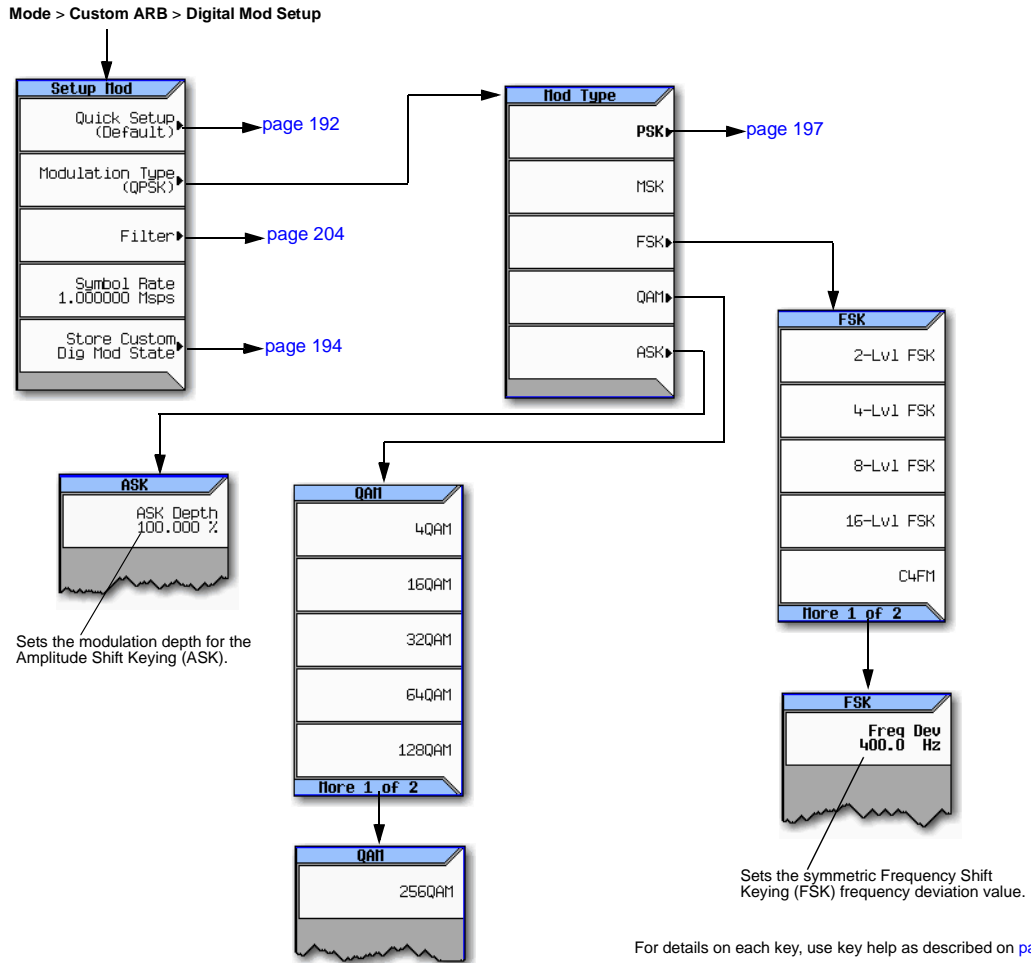


Figure 11-4 Store Custom Dig Mod Softkeys

Mode > Custom ARB > Digital Mod Setup > Store Custom Dig Mod State

The screenshot shows the 'Store Custom Dig Mod State' screen. At the top, it displays 'FREQUENCY 6.000 000 000 00 GHz' and 'AMPLITUDE -144.00 dBm'. Below this is a 'Catalog of DMOD Files in Int Storage' with 29.6MB used and 468MB free. The catalog lists one file: '1 FIR_EXAM' of type 'DMOD', size '312', and modified '01/24/07 14:22'. The bottom right corner shows the date and time '01/24/2007 16:56'. On the right side, there are three softkey options: 'Store To File', 'Delete File', and 'Goto Row'. Arrows point from these softkeys to callout boxes: 'Store To File' points to a 'Confirm Delete' dialog, 'Delete File' points to another 'Confirm Delete' dialog, and 'Goto Row' points to a 'Goto Row' dialog with options for 'Enter', 'Goto Top Row', 'Goto Middle Row', and 'Goto Bottom Row'. A blue arrow points from the top right of the screen to 'page 199'. A text box at the bottom explains that the catalog displays digital modulation (DMOD) files that have been previously saved.


Catalog displays digital modulation (DMOD) files that have been previously saved.

For details on each key, use key help as described on [page 26](#).

Using the Arbitrary Waveform Generator

This section teaches you how to build dual arbitrary (ARB) waveform files containing custom TDMA, digital modulation for testing component designs.

Figure 11-5 Adding Custom Modulation to a Waveform

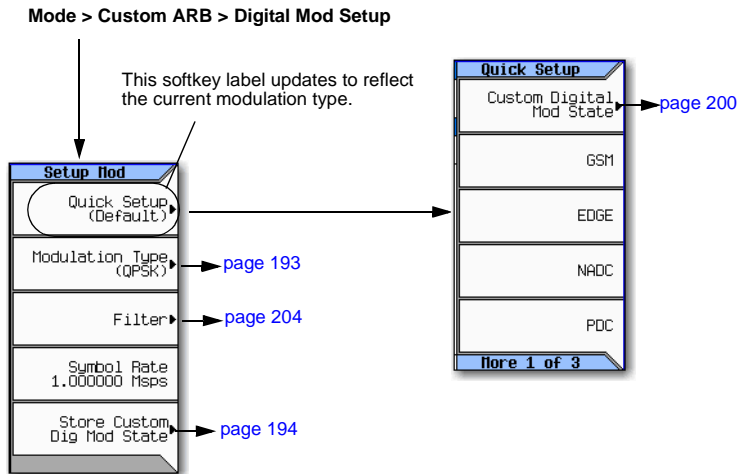

For details on each key, use key help as described on [page 26](#).

Using Predefined Custom TDMA Digital Modulation

This section teaches you how to perform the following tasks:

- [Selecting a Predefined EDGE Setup](#) on page 195
- [Generating the Waveform](#) on page 195
- [Configuring the RF Output](#) on page 196

Selecting a Predefined EDGE Setup

1. Press **Preset**.
2. In the Custom ARB menu ([page 195](#)), press **Digital Mod Setup > Quick Setup > EDGE**.

Generating the Waveform

Press **Digital Modulation Off On**.

This generates a waveform with the pre-defined EDGE state selected in the step. The display changes to Dig Mod Setup: EDGE. During waveform generation, the DIGMOD and I/Q annunciators appear and the pre-defined digital modulation state is stored in volatile memory (BBG). The waveform is now modulating the RF carrier.

Configuring the RF Output

1. Set the RF output frequency to 891 MHz.
2. Set the output amplitude to -5 dBm.
3. Press **RF On/Off**.


The predefined EDGE signal is now available at the signal generator's RF OUTPUT connector.

Creating a Custom TDMA Digital Modulation State

In this procedure, you learn how to set up a single-carrier NADC digital modulation with customized modulation type, symbol rate, and filtering.

Figure 11-6 Modifying a Digital Modulation Type

Mode > Custom ARB > Digital Mod Setup

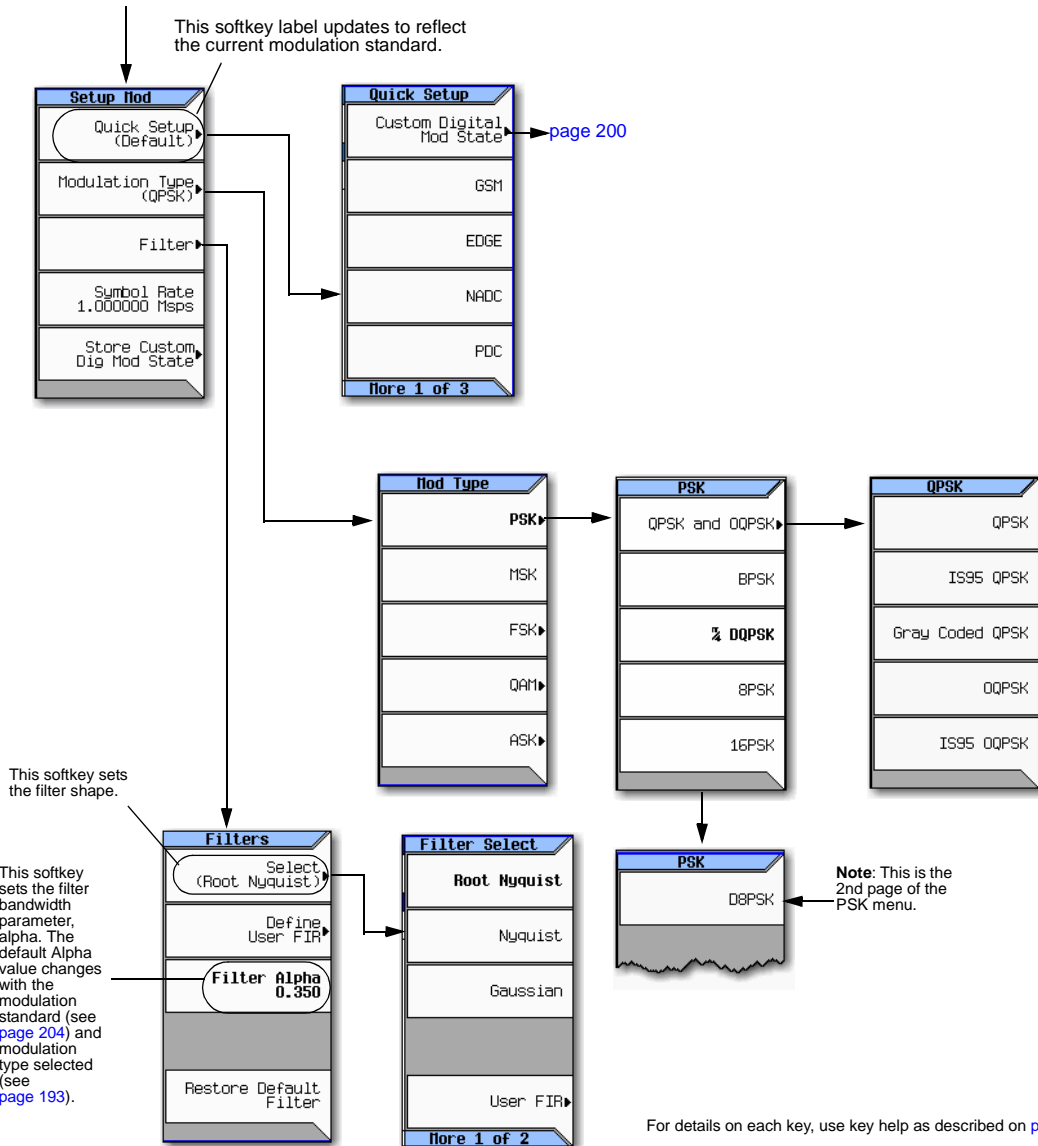

This section teaches you how to perform the following tasks:

- [Selecting a Digital Modulation Setup](#) on page 198
- [Configuring the RF Output](#) on page 196
- [Selecting the Filter](#) on page 198
- [Configuring the RF Output](#) on page 196

Selecting a Digital Modulation Setup

1. Press **Preset**.
2. In the Custom Arb menu ([page 197](#)), press **Digital Mod Setup > Quick Setup > NADC**.

Modifying the Modulation Type and Symbol Rate

1. In the Custom ARB menu ([page 197](#)), press **Digital Mod Setup > Modulation Type > PSK > QPSK and OQPSK > QPSK**.
2. Press **Symbol Rate > 56 > ksps**.

Selecting the Filter

1. In the Setup Mod menu ([page 197](#)), press **Filter > Select > Nyquist**.
2. Press **Return > Return**.

Generating the Waveform

Press **Digital Modulation Off On**.

This generates a waveform with the custom, single-carrier NADC, digital modulation state created in the previous sections. The display changes to Dig Mod Setup: NADC (Modified). During waveform generation, the DIGMOD and I/Q annunciators appear and the custom single-carrier digital modulation state is stored in volatile memory. The waveform is now modulating the RF carrier.

For instructions on storing this custom, single-carrier NADC, digital modulation state to the non-volatile memory catalog, see [Storing a Custom TDMA Digital Modulation State](#) on page 198.

Configuring the RF Output

1. Set the RF output frequency to 835 MHz.
2. Set the output amplitude to 0 dBm.
3. Press **RF On/Off**.


The user-defined NADC signal is now available at the RF OUTPUT connector.

Storing a Custom TDMA Digital Modulation State

Using this procedure, you learn how to store a custom digital modulation state and a custom multicarrier digital modulation state to non-volatile memory.

If you have not created a custom, single-carrier, digital modulation state, complete the steps in the previous section, [Creating a Custom TDMA Digital Modulation State](#) on page 197.

Figure 11-7 Storing a Custom Digital Modulation State

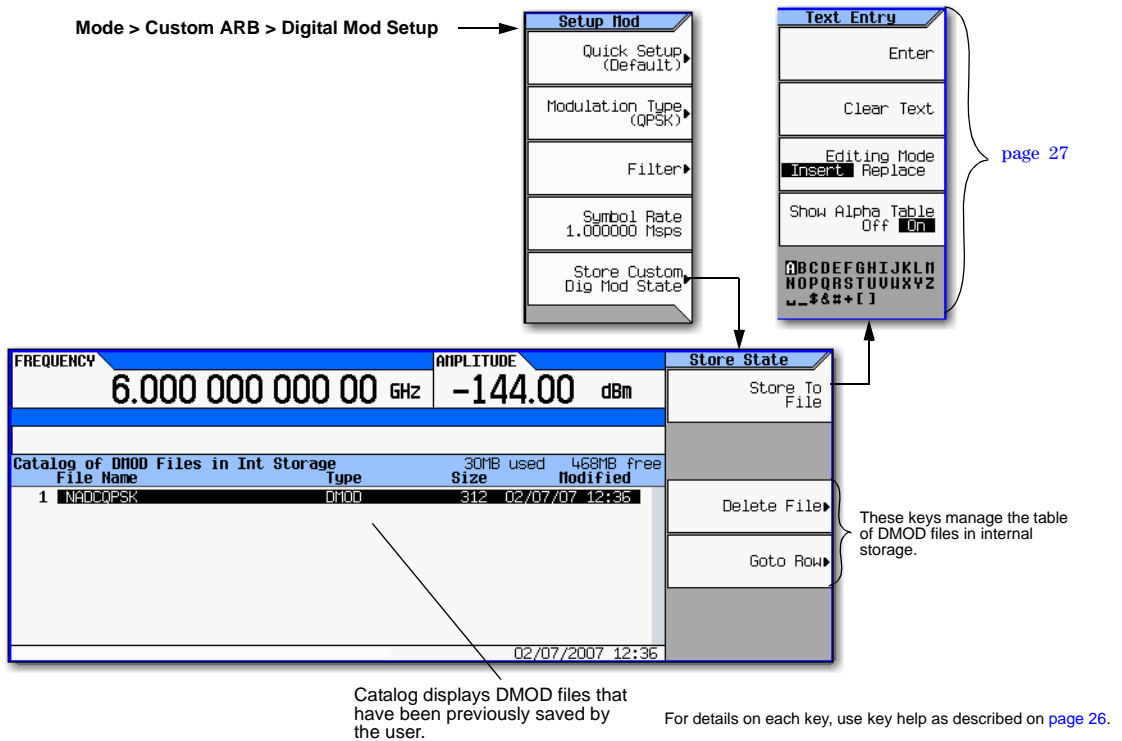

1. Return to the top-level Custom ARB menu, where **Digital Modulation Off On** is the first softkey.
2. In the Custom ARB menu (page 199), press **Digital Mod Setup > Store Custom Dig Mod State > Store To File**.

If there is already a file name from the Catalog of DMOD Files occupying the active entry area, press the following key: **Clear Text**

3. Enter a file name (for example, NADCQPSK) using the alpha keys and the numeric keypad with a maximum length of 23 characters.
4. Press **Enter**.

The user-defined, single-carrier, digital modulation state is now stored in non-volatile memory.

NOTE The RF output amplitude, frequency, and operating state settings are not stored as part of a user-defined, digital modulation state file.


Recalling a Custom TDMA Digital Modulation State

Using this procedure, you will learn how to recall a custom digital modulation state from signal non-volatile memory.

If you have not created and stored a user-defined, single-carrier, digital modulation state, complete the steps in the previous sections, [Creating a Custom TDMA Digital Modulation State](#) on page 197 and [Storing a Custom TDMA Digital Modulation State](#) on page 198, then preset the signal generator to clear the stored user-defined, digital modulation waveform from volatile ARB memory.

Figure 11-8 Recalling a Custom TDMA Digital Modulation State

Mode > Custom ARB > Digital Mod Setup > Quick Setup

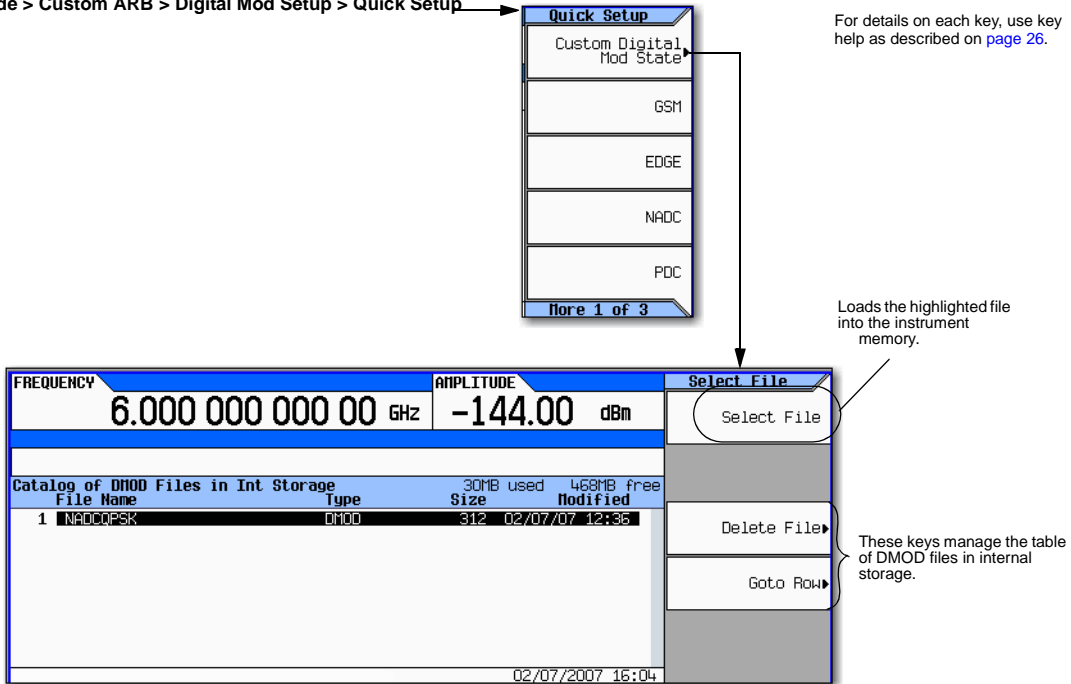

1. In the Quick Setup menu, press **Custom Digital Mod State**.
2. Highlight the desired file (for example, NADCQPSK).
3. Press **Select File > Return**.
4. Press **Digital Modulation Off On** until On is highlighted.

The instrument regenerates the custom, digital modulation waveform in volatile memory. After waveform generation, the custom, digital modulation waveform is available to be modulated on the RF output.

For instruction on configuring the RF output, see [Configuring the RF Output](#) on page 196.


Creating a Custom Multicarrier TDMA Digital Modulation State

In this procedure, you learn how to customize a predefined, multicarrier, digital modulation setup by creating a custom, 3-carrier EDGE, digital modulation state.

This section teaches you how to perform the following tasks:

- “Creating a Multicarrier Digital Modulation Setup” on page 201
- “Modifying Carrier Frequency Offset” on page 202
- “Modifying Carrier Power” on page 202
- “Generating the Waveform” on page 202
- “Configuring the RF Output” on page 202

Figure 11-9 Creating a Multicarrier Digital Modulation Setup

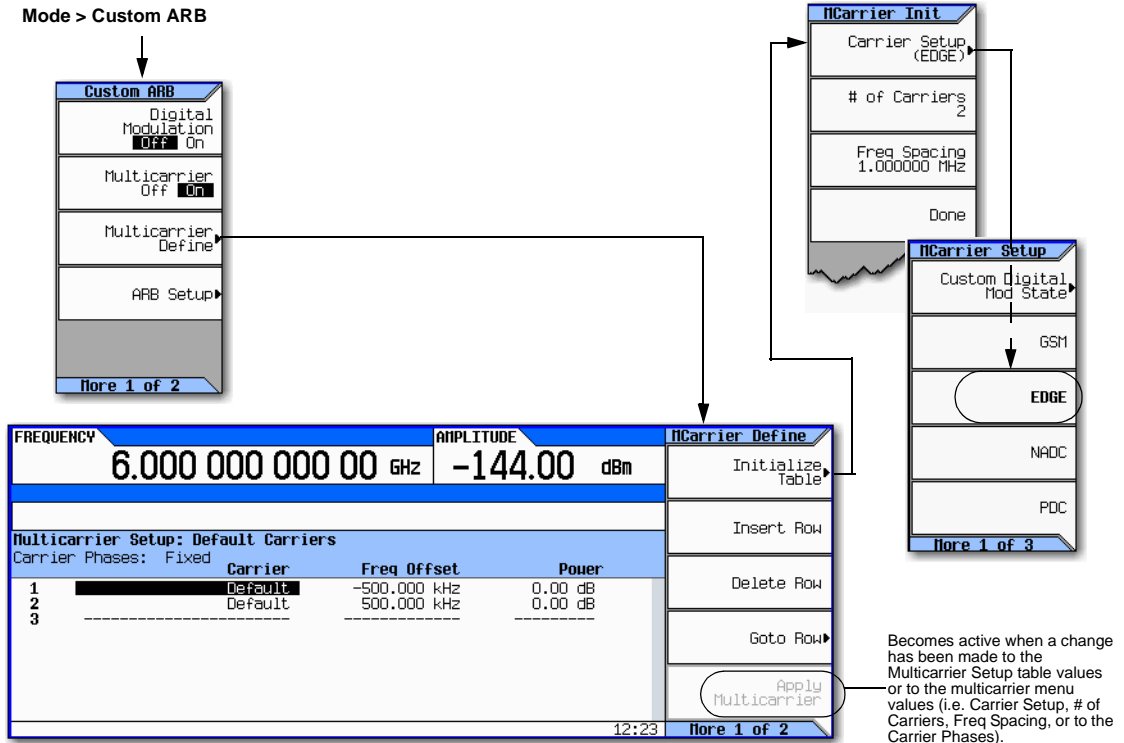

For details on each key, use key help as described on page 26.

Creating a Multicarrier Digital Modulation Setup

1. Press **Preset**.

2. Press **Mode** > **Custom ARB** > **Multicarrier Off On** to **On**.
3. Press **Multicarrier Define** > **Initialize Table** > **Carrier Setup** > **EDGE** > **Done**.

Modifying Carrier Frequency Offset

1. Highlight the Freq Offset value (500.000 kHz) for the carrier in row 2.
2. Press **-625** > **kHz**.

Modifying Carrier Power

1. Highlight the Power value (0.00 dB) for the carrier in row 2.
2. Press **-10** > **dB**.

You now have a custom 2-carrier EDGE waveform with a carrier at a frequency offset of -625 kHz and a power level of -10.00 dBm, as shown in the following figure.

FREQUENCY	AMPLITUDE	Carrier Define
6.000 000 000 00 GHz	-144.00 dBm	Initialize Table
Multicarrier Setup: EDGE Carriers (Modified)		
Carrier Phases: Fixed		
Carrier	Freq Offset	Power
1 EDGE	-500.000 kHz	0.00 dB
2 EDGE	-625.000 kHz	-10.00 dB
3 -----		

For details on each key, use key help as described on [page 26](#).

If Digital Modulation is already on, you must press Apply Multicarrier to apply the changes and generate a new custom multicarrier digital modulation waveform based on the updated values.

Generating the Waveform

Press **Return** > **Digital Modulation Off On**.

This generates a waveform with the custom, multicarrier, EDGE state created in the previous sections. The display changes to Dig Mod Setup: Multicarrier (Modified). During waveform generation, the DIGMOD and I/Q annunciators appear and the new custom, multicarrier, EDGE state is stored in volatile memory. The waveform is now modulating the RF carrier.

For instructions on storing this custom, multicarrier, EDGE state to non-volatile memory, see [“Storing a Custom Multicarrier TDMA Digital Modulation State” on page 203](#).

Configuring the RF Output

1. Set the RF output frequency to 890.01 MHz.
2. Set the output amplitude to -10 dBm.
3. Press **RF On/Off**.

The custom multicarrier EDGE signal is now available at the RF OUTPUT connector.

Storing a Custom Multicarrier TDMA Digital Modulation State

Using this procedure, you learn how to store a custom, multicarrier, TDMA, digital modulation state to non-volatile memory.

If you have not created a custom, multicarrier, digital modulation state, complete the steps in the previous section, “Creating a Custom Multicarrier TDMA Digital Modulation State” on page 201.

Figure 11-10 Storing a Custom Multicarrier Softkeys

The screenshot shows the 'Carrier Define' menu with the following details:

- FREQUENCY:** 6.000 000 000 00 GHz
- AMPLITUDE:** -144.00 dBm
- Carrier Phases:** Fixed (selected), Random
- Multicarrier Setup: EDGE Carriers (Modified)**

Carrier	Carrier	Freq Offset	Power
1	EDGE	-500.000 kHz	0.00 dB
2	EDGE	-625.000 kHz	-10.00 dB
3	-----	-----	-----
- Softkeys:** Carrier Phases, Load/Store, Edit Item
- Footer:** 02/21/2007 17:22, Page 2 of 2

Annotations on the right side of the image:

- Fixed: All the carriers are set to a phase of 0.
- Random: All of the carriers are set to a random phase value.
- Load/Store: page 27
- For details on each key, use key help as described on page 26.

1. Return to the top-level Digital Modulation menu, where **Digital Modulation Off On** is the first softkey.
2. Press **Multicarrier Define > More > Load/ Store > Store To File**.

If there is already a file name from the Catalog of MDMOD Files occupying the active entry area, press the following key: **Clear Text**

3. Enter a file name (for example, EDGEM1) using the alpha keys and the numeric keypad with a maximum length of 23 characters.
4. Press **Enter**.

The user-defined, multicarrier, digital modulation state is now stored in non-volatile memory.

NOTE The RF output amplitude, frequency, and operating state settings are not stored as part of a user-defined, digital modulation state file.

Applying Changes to an Active Multicarrier TDMA Digital Modulation State

If the digital modulation format is currently in use (**Digital Modulation Off On** set to On) while changes are made in the Multicarrier Setup table editor, you must apply the changes before the updated waveform will be generated.


From the Multicarrier Setup table editor, press **Apply Multicarrier** to apply the changes and generate a new custom multicarrier digital modulation waveform based on the updated values.

Using Finite Impulse Response (FIR) Filters

Finite Impulse Response filters can be used to refine the symbol of the generated waveforms.

Figure 11-11 Filter Menu

Mode > Custom ARB > Digital Mod Setup > Filter

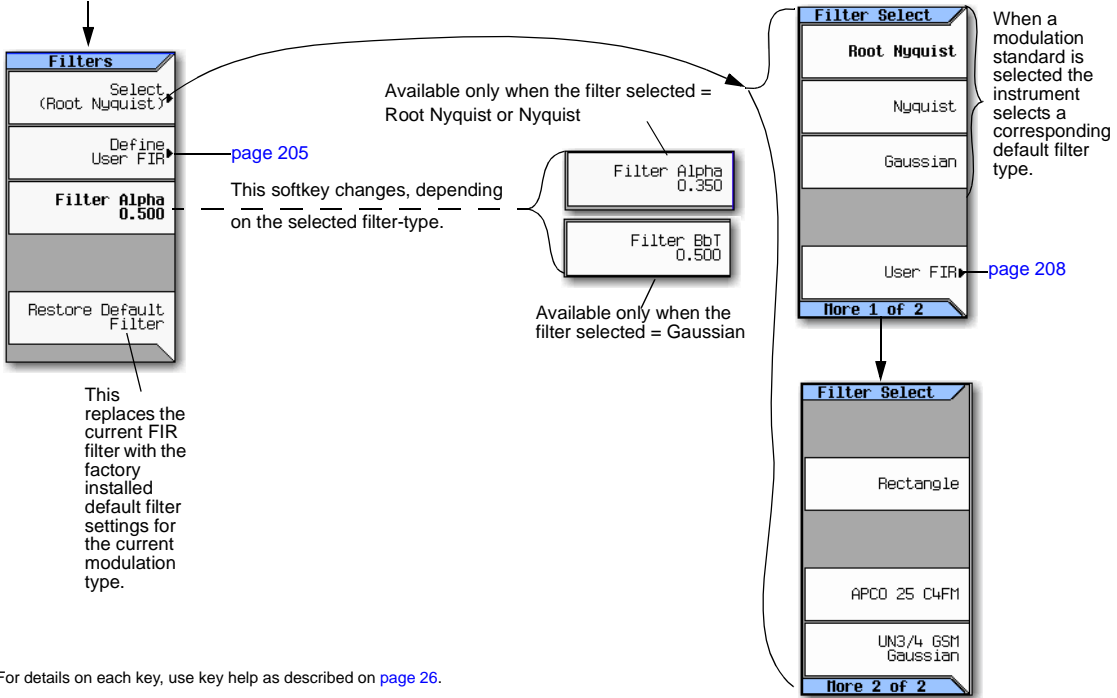

For details on each key, use key help as described on page 26.

Creating a User-Defined FIR Filter Using the FIR Table Editor

In this procedure, you use the FIR Values table editor to create and store an 8-symbol, windowed sync function filter with an oversample ratio of 4.

Accessing the Table Editor


1. Press **Preset**.
2. Press **Mode > Custom ARB > Digital Mod Setup > Quick Setup > NADC**.
3. Press **Filter > Define User FIR**.
4. Press **More 1 of 2 > Delete All Rows > Confirm Delete of All Rows**.

This will initialize the table editor as shown in Figure 11-12.

Figure 11-12 Creating a User-Defined FIR Filter Using the FIR Filter Table Editor

Mode > Custom ARB > Digital Mod Setup > Filter > Define User FIR >
More 1 of 2 > Delete All Rows > Confirm Delete of All Rows

For details on each key, use key help as described on [page 26](#).

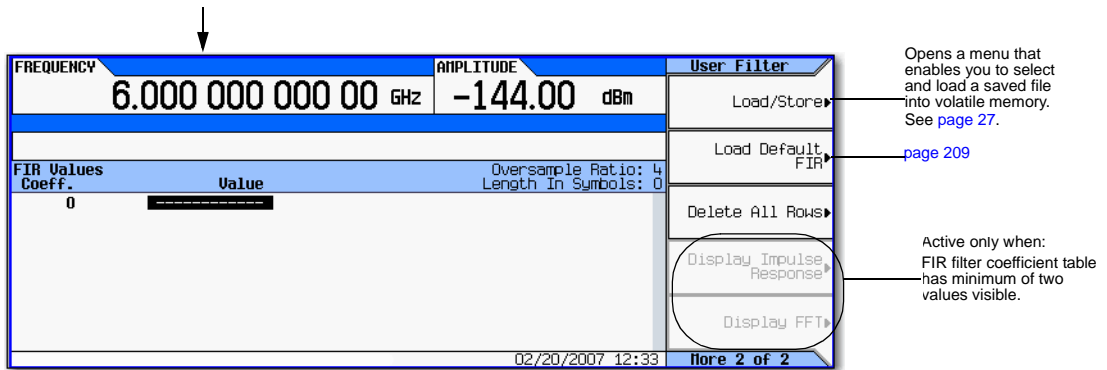

Entering the Coefficient Values

1. Press the **Return** softkey to get to the first page of the table editor.
2. Use the cursor to highlight the Value field for coefficient 0.
3. Use the numeric keypad to type the first value (−0.000076) from [Table 11-1](#). As you press the numeric keys, the numbers are displayed in the active entry area. (If you make a mistake, you can correct it using the backspace key.)
4. Continue entering the coefficient values from the table in step 1 until all 16 values have been entered.

Table 11-1

Coefficient	Value
0	−0.000076
1	−0.001747
2	−0.005144
3	−0.004424
4	0.007745
5	0.029610
6	0.043940
7	0.025852

Coefficient	Value
8	−0.035667
9	−0.116753
10	−0.157348
11	−0.088484
12	0.123414
13	0.442748
14	0.767329
15	0.972149


Duplicating the First 16 Coefficients Using Mirror Table

In a windowed sinc function filter, the second half of the coefficients are identical to the first half in reverse order. The signal generator provides a mirror table function that automatically duplicates the existing coefficient values in the reverse order.

1. Press **Mirror Table**. The last 16 coefficients (16 through 31) are automatically generated and the first of these coefficients (number 16) highlights, as shown in [Figure 11-13 on page 206](#).

Figure 11-13

FIR table coefficient values, may be from the factory default values or entered by the user.

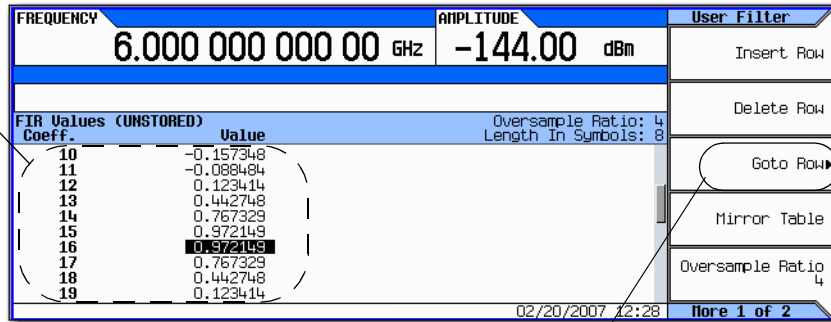

Use the Goto Row menu to move around and make changes to the FIR Values coefficient table.

For details on each key, use key help as described on [page 26](#).

Setting the Oversample Ratio

The oversample ratio (OSR) is the number of filter coefficients per symbol. Acceptable values range from 1 through 32; the maximum combination of symbols and oversampling ratio allowed by the table editor is 1024. The instrument hardware, however, is actually limited to 32 symbols, an oversample ratio between 4 and 16, and 512 coefficients. So if you enter more than 32 symbols or 512 coefficients, the instrument is unable to use the filter. If the oversample ratio is different from the internal, optimally selected one, then the filter is automatically resampled to an optimal oversample ratio.

For this example, the desired OSR is 4, which is the default, so no action is necessary.


Displaying a Graphical Representation of the Filter

The signal generator has the capability of graphically displaying the filter in both time and frequency dimensions.

1. Press **More 1 of 2 > Display FFT** (fast Fourier transform).

Refer to [Figure 11-14 on page 207](#).

Figure 11-14

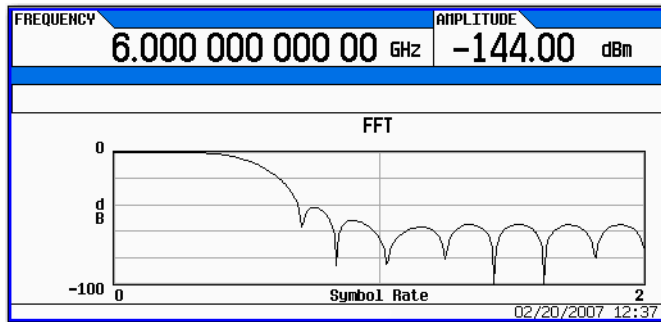


For details on each key, use key help as described on [page 26](#).

2. Press **Return**.
3. Press **Display Impulse Response**.

Refer to [Figure 11-15](#).

Figure 11-15

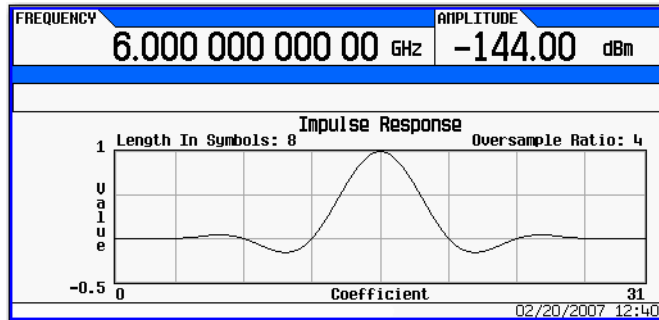

For details on each key, use key help as described on [page 26](#).

4. Press **Return** to return to the menu keys.


Storing the Filter to Memory

Use the following steps to store the file.

1. Press **Load/Store > Store To File**. The catalog of FIR files appears along with the amount of memory available.
2. As described in [Storing, Loading, and Playing a Waveform Segment](#) on page 98, name and store this file as **FIR_1**.

The **FIR_1** file is the first file name listed. (If you have previously stored other FIR files, additional file names are listed below **FIR_1**.) The file type is **FIR** and the size of the file is 260 bytes. The amount of memory used is also displayed. The number of files that can be saved depends on the size of the files and the amount of memory used. Refer to [Figure 11-16](#).

Figure 11-16

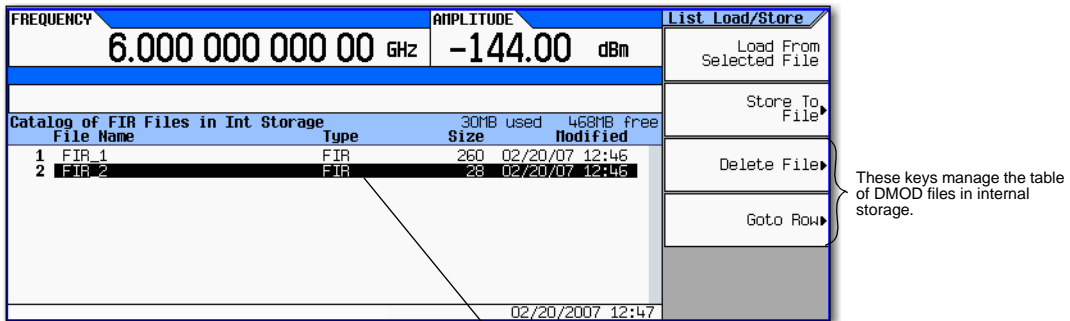

Catalog displays FIR files that have been previously saved by the user.

For details on each key, use key help as described on page 26.

Memory is also shared by instrument state files and list sweep files.

This filter can now be used to customize a modulation format or it can be used as a basis for a new filter design.

Modifying a FIR Filter Using the FIR Table Editor


FIR filters stored in signal generator memory can easily be modified using the FIR table editor. You can load the FIR table editor with coefficient values from user-defined FIR files stored in non-volatile memory or from one of the default FIR filters. Then you can modify the values and store the new files.

Loading the Default Gaussian FIR File

Figure 11-17 Loading the Default Gaussian FIR File

Mode > Custom ARB > Digital Mod Setup

For details on each key, use key help as described on [page 26](#).

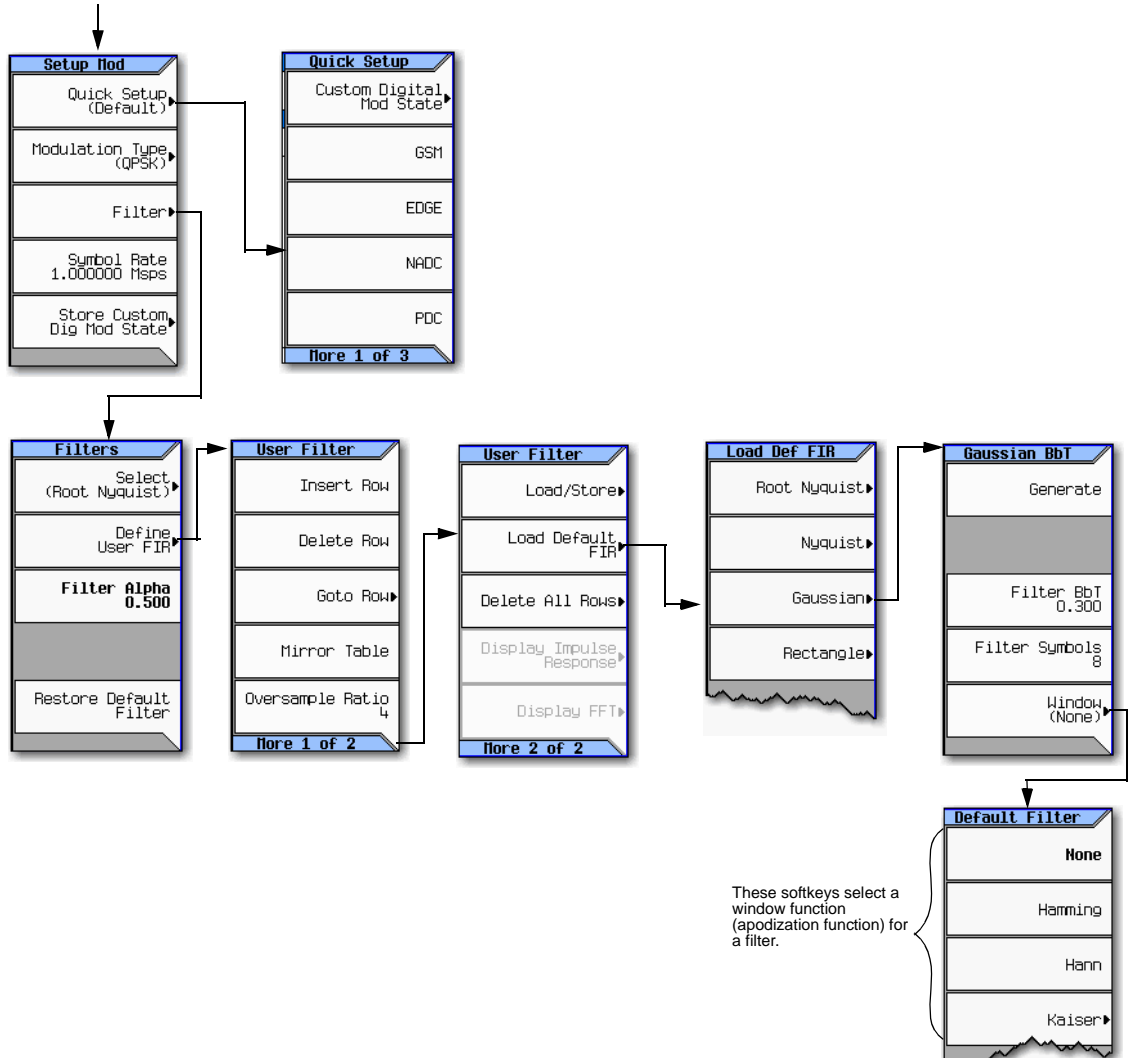


1. Press **Preset**.
2. Press **Mode > Custom ARB > Digital Mod Setup > Quick Setup > NADC**.
3. Press **Filter > Define User FIR > More 1 of 2 > Load Default FIR > Gaussian**.
4. Press **Filter BbT > 0.300 > Enter**.

5. Press **Filter Symbols > 8 > Enter**.
6. Press **Generate**.

NOTE The actual oversample ratio during modulation is automatically selected by the instrument. A value between 4 and 16 is chosen dependent on the symbol rate, the number of bits per symbol of the modulation type, and the number of symbols.

7. Press **Display Impulse Response** (refer to [Figure 11-18](#)).

Figure 11-18

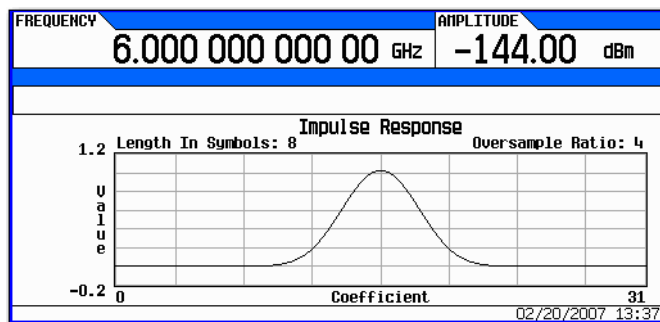


For details on each key, use key help as described on [page 26](#).

8. Press **Return**.

Modifying the Coefficients

1. Using the front-panel arrow keys, highlight coefficient 15.
2. Press **0 > Enter**.
3. Press **Display Impulse Response**.

Figure 11-19

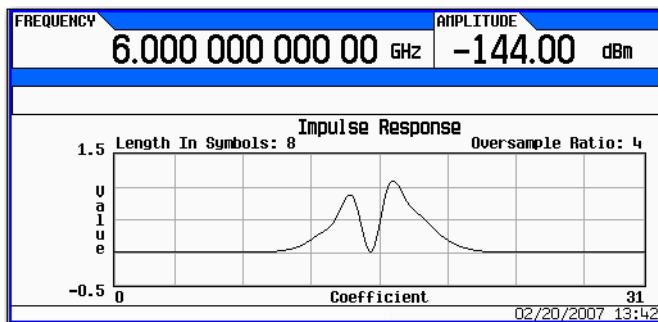

For details on each key, use key help as described on [page 26](#).

Refer to [Figure 11-19 on page 210](#). The graphic display can provide a useful troubleshooting tool (in this case, it indicates that a coefficient value is missing, resulting in an improper Gaussian response).

4. Press **Return**.
5. Highlight coefficient 15.
6. Press **1 > Enter**.

Storing the Filter to Memory

The maximum file name length is 23 characters (alphanumeric and special characters).

1. Press **Load/Store > Store To File**.
2. Name the file NEWFIR2.
3. Press **Enter**.

The contents of the current FIR table editor are stored to a file in non-volatile memory and the catalog of FIR files is updated to show the new file.

12 Multitone and Two-Tone Waveform Generator (Option 430)

Before using this information, you should be familiar with the basic operation of the signal generator. If you are not comfortable with functions such as setting the power level and frequency, refer to [Basic Operation](#) on page 25 and familiarize yourself with the information in that chapter.

This feature is available only in N5182A Agilent MXG Vector Signal Generators with Option 430. Option 430 requires Option 651, 652, or 654.

Creating a Custom Two-Tone Waveform

Using the Two-Tone menu, you can define, and modify user-defined Two-Tone waveforms. Two-Tone waveforms are generated by the dual arbitrary waveform generator.

The section [Using Two-Tone Modulation](#) on page 214 teaches you how to perform the following tasks:

- [Creating a Two-Tone Waveform](#) on page 215
- [Viewing a Two-Tone Waveform](#) on page 216
- [Minimizing Carrier Feedthrough](#) on page 217
- [Changing the Alignment of a Two-Tone Waveform](#) on page 218

Creating a Custom Multitone Waveform

Using the Multitone Setup table editor, you can define, modify and store user-defined multitone waveforms. Multitone waveforms are generated by the dual arbitrary waveform generator.

The [Using Multitone Modulation](#) on page 220 teaches you how to perform the following tasks:

- [Initializing the Multitone Setup Table Editor](#) on page 220
- [Configuring Tone Powers and Tone Phases](#) on page 221
- [Removing a Tone](#) on page 221
- [Generating the Waveform](#) on page 221
- [Configuring the RF Output](#) on page 222

Using Two-Tone Modulation


In the following sections, this chapter describes the two-tone mode, which is available only in N5182A Agilent MXG Vector signal generators with Option 430:

- [Creating a Two-Tone Waveform](#) on page 215
- [Viewing a Two-Tone Waveform](#) on page 216
- [Minimizing Carrier Feedthrough](#) on page 217
- [Changing the Alignment of a Two-Tone Waveform](#) on page 218

See also: [Saving a Waveform's Settings & Parameters](#) on page 105

NOTE For more information about two-tone waveform characteristics, and the two-tone standard, download *Application Note 1410* from our website by going to <http://www.agilent.com> and searching for “AN 1410” in Test & Measurement.

Two Tone Modulation Softkeys

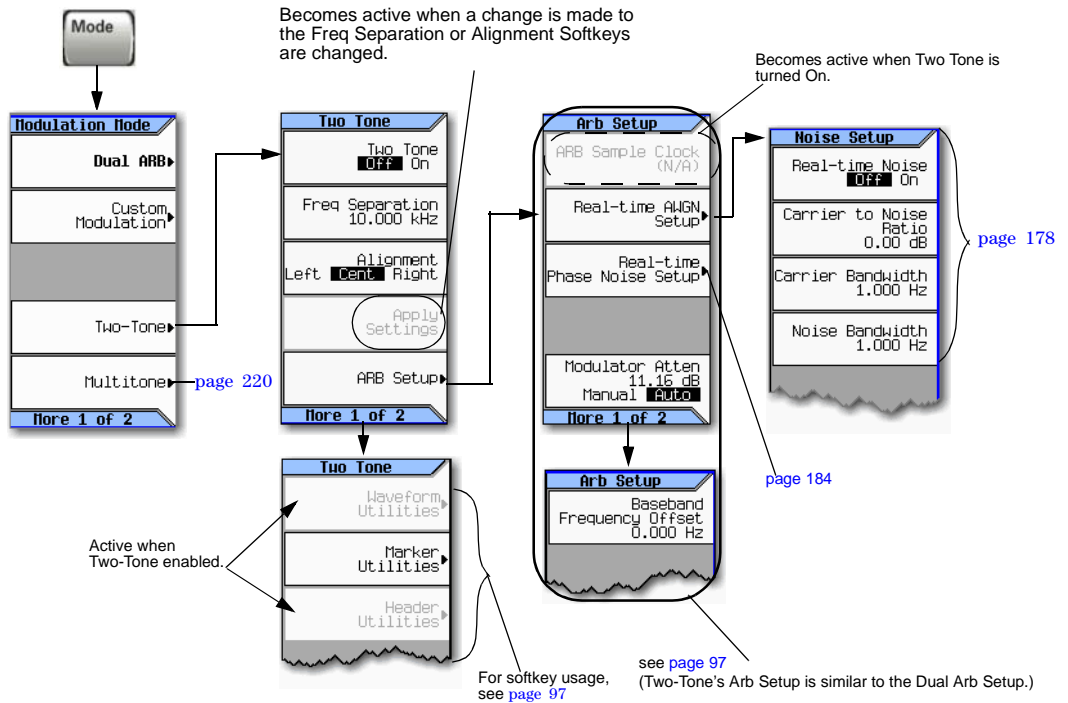

For details on each key, use key help as described on page 26.


Creating a Two-Tone Waveform

This procedure describes how to create a basic, centered, two-tone waveform.

1. Preset the signal generator.
2. Set the signal generator RF output frequency to 6 GHz.
3. Set the signal generator RF output amplitude to -10 dBm.
4. Press **Mode** > **Two-Tone** > **Freq Separation** > **10** > **MHz**.
5. Press **Two Tone Off On** to On.
6. Turn on the RF output.

The two-tone signal is now available at the signal generator RF OUTPUT connector. [Figure 12-1 on page 216](#) shows what the signal generator display should look like after all steps have been completed. Notice that the T-TONE, I/Q, annunciators are displayed; the RF ON, MOD ON LEDs are on; and the parameter settings for the signal are shown in the status area of the signal generator display.

Figure 12-1

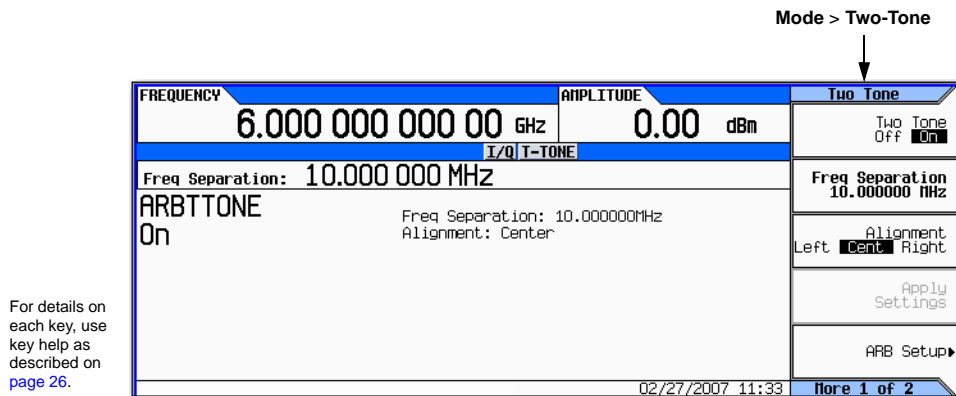


Viewing a Two-Tone Waveform

This procedure describes how to configure the spectrum analyzer to view a two-tone waveform and its IMD products. Actual key presses will vary, depending on the model of spectrum analyzer you are using.

1. Preset the spectrum analyzer.
2. Set the carrier frequency to 6 GHz.
3. Set the frequency span to 60 MHz.
4. Set the amplitude for a 10 dB scale with a -10 dBm reference.
5. Adjust the resolution bandwidth to sufficiently reduce the noise floor to expose the IMD products. A 9.1 kHz setting was used in our example.
6. Turn on the peak detector.
7. Set the attenuation to 4 dB, so you're not overdriving the input mixer on the spectrum analyzer.

You should now see a two-tone waveform with a 6 GHz center carrier frequency that is similar to the one shown in [Figure 12-2 on page 217](#). You will also see IMD products at 10 MHz intervals above and below the generated tones, and a carrier feedthrough spike at the center frequency with carrier feedthrough distortion products at 10 MHz intervals above and below the center carrier frequency.

Figure 12-2

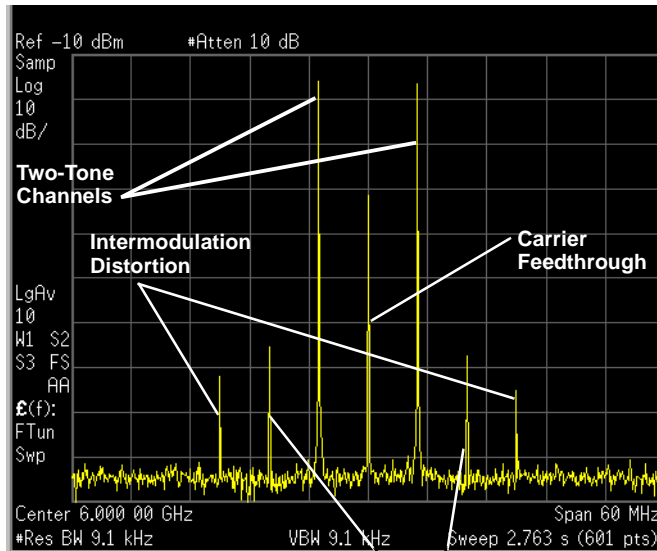

For details on each key, use key help as described on [page 26](#).

Carrier Feedthrough
Distortion

Minimizing Carrier Feedthrough

This procedure describes how to minimize carrier feedthrough and measure the difference in power between the tones and their intermodulation distortion products. Before beginning this procedure, it is important that a recent I/Q calibration has been performed on the instrument. The procedure for performing an I/Q calibration (refer to “[I/Q Calibration](#)” on [page 157](#)).

This procedure builds upon the previous procedure.


1. On the spectrum analyzer, set the resolution bandwidth for a sweep rate of about 100-200 ms. This will allow you to dynamically view the carrier feedthrough spike as you make adjustments.
2. On the signal generator, press **I/Q > I/Q Adjustments > I/Q Adjustments Off On** to On.
3. Press **Internal Baseband Adjustments > I Offset** and turn the rotary knob while observing the carrier feedthrough with the spectrum analyzer. Changing the I offset in the proper direction will reduce the feedthrough level. Adjust the level as low as possible.
4. Press **Q Offset** and turn the rotary knob to further reduce the carrier feedthrough level.
5. Repeat steps 3 and 4 until you have reached the lowest possible carrier feedthrough level.
6. On the spectrum analyzer, return the resolution bandwidth to its previous setting.
7. Turn on waveform averaging.

8. Create a marker and place it on the peak of one of the two tones.
9. Create a delta marker and place it on the peak of the adjacent intermodulation product, which should be spaced 10 MHz from the marked tone.
10. Measure the power difference between the tone and its distortion product.

You should now see a display that is similar to the one shown in [Figure 12-3 on page 218](#). Your optimized two-tone signal can now be used to measure the IMD products generated by a device-under-test.

Note that carrier feedthrough changes with time and temperature. Therefore, you will need to periodically readjust your I and Q offsets to keep your signal optimized.

Figure 12-3

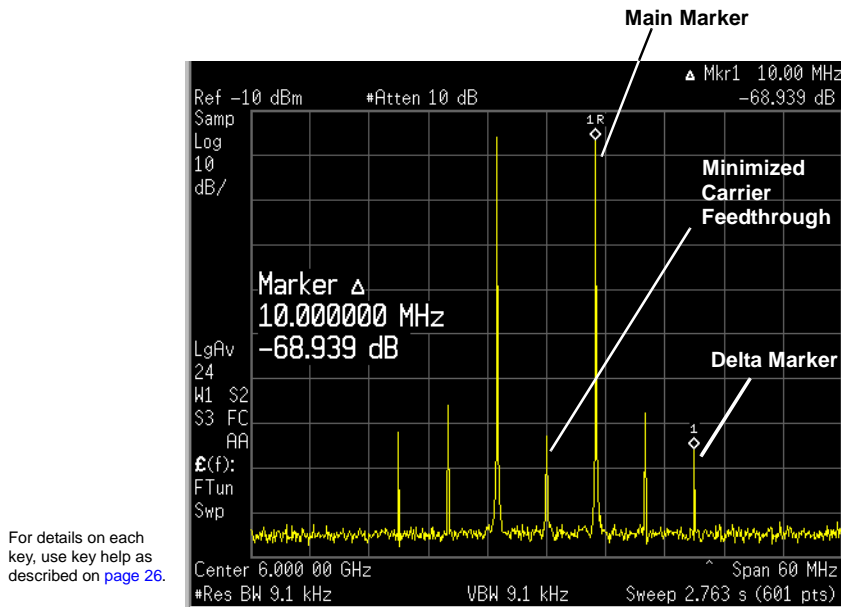

Changing the Alignment of a Two-Tone Waveform


This procedure describes how to align a two-tone waveform left or right, relative to the center carrier frequency. Because the frequency of one of the tones is the same as the carrier frequency, this alignment typically hides any carrier feedthrough. However, image frequency interference caused by left or right alignment may cause minor distortion of the two-tone signal. This procedure builds upon the previous procedure.

1. On the signal generator, press **Mode > Two Tone > Alignment Left Cent Right** to Left.
2. Press **Apply Settings** to regenerate the waveform.

NOTE Whenever a change is made to a setting while the two-tone generator is operating (**Two Tone Off On** set to On), you must apply the change by pressing the **Apply Settings** softkey before the updated waveform will be generated. When you apply a change, the baseband generator creates a two-tone waveform using the new settings and replaces the existing waveform in ARB memory.

3. On the spectrum analyzer, temporarily turn off waveform averaging to refresh your view more quickly. You should now see a left-aligned two-tone waveform that is similar to the one shown in [Figure 12-4](#).


Figure 12-4

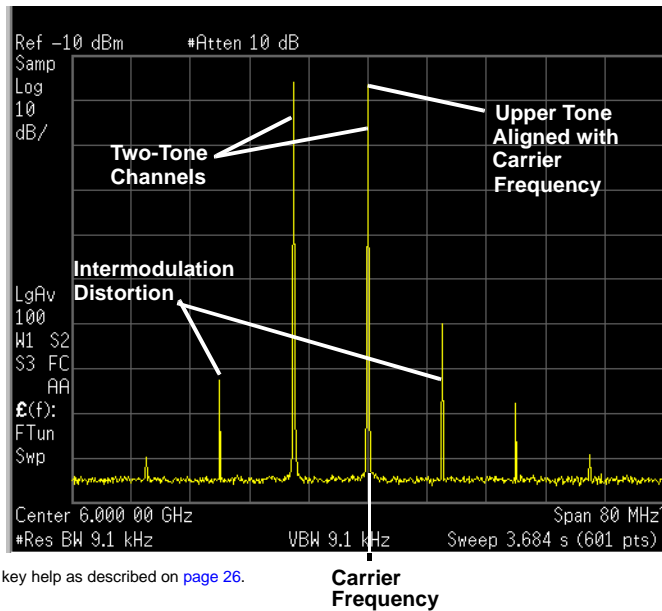

For details on each key, use key help as described on [page 26](#).

Using Multitone Modulation

Multitone Modulation Softkeys

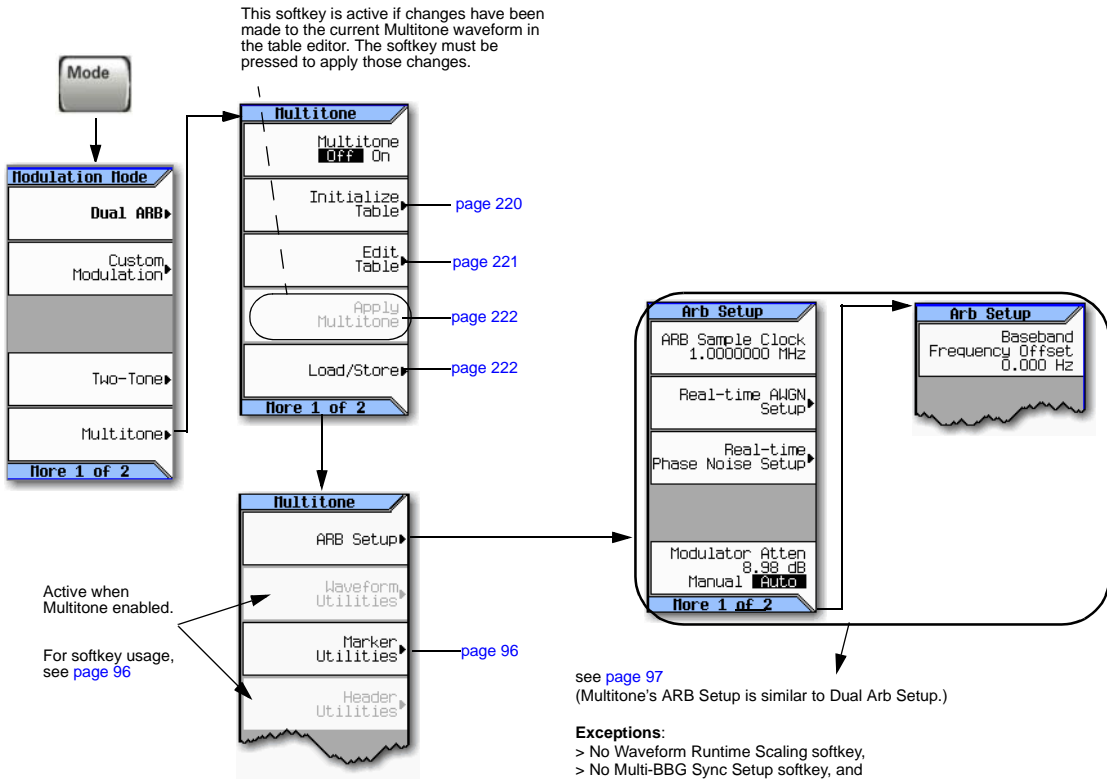


For details on each key, use key help as described on page 26.

Initializing the Multitone Setup Table Editor

1. Press **Preset**.
2. Press **Mode > Multitone**
3. Press **Initialize Table > Number of Tones > 5 > Enter**.
4. Press **Freq Spacing > 20 > kHz**.

Figure 12-5

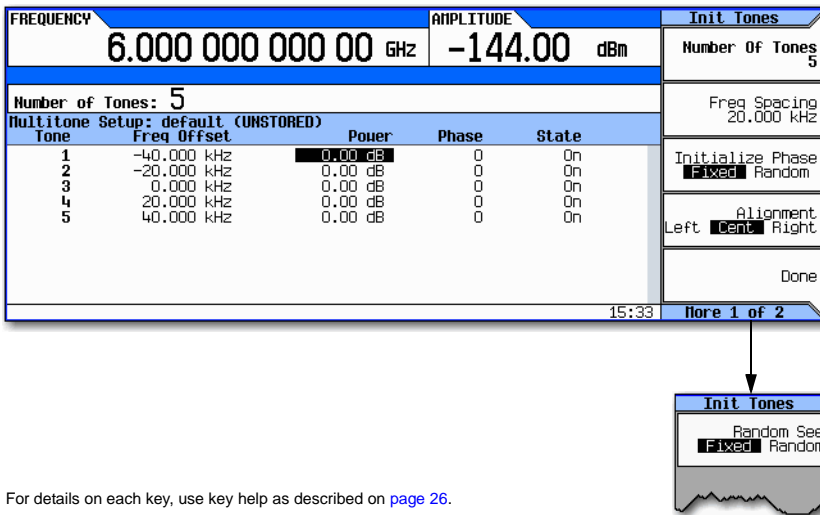

For details on each key, use key help as described on page 26.

5. Press **Done**.

You now have a multitone setup with five tones spaced 20 kHz apart. The center tone is placed at the carrier frequency, while the other four tones are spaced in 20 kHz increments from the center tone.

Configuring Tone Powers and Tone Phases

1. Highlight the value (0 dB) in the Power column for the tone in row 2.
2. Press **Edit Table > Edit Item > -4.5 > dB**.
3. Highlight the value (0) in the Phase column for the tone in row 2.
4. Press **Edit Item > 123 > deg**.

Removing a Tone

1. Highlight the value (On) in the State column for the tone in row 4.
2. Press **Toggle State**.

Generating the Waveform

Press **Return > Multitone Off On** until On is highlighted.

This generates the multitone waveform with the parameters defined in the previous sections. During waveform generation, the M-TONE and I/Q annunciators activate and the multitone waveform is stored in volatile ARB memory. The waveform is now modulating the RF carrier.

Configuring the RF Output

1. Set the RF output frequency to 100 MHz.
2. Set the output amplitude to 0 dBm.
3. Press **RF On/Off**.

The multitone waveform is now available at the signal generator's RF OUTPUT connector.

Applying Changes to an Active Multitone Signal

If the multitone generator is currently in use (**Multitone Off On** set to On) while changes are made in the Multitone Setup table editor, you must *apply* the changes before the updated waveform will be generated.

From the Multitone Setup table editor, press the following key to apply the changes and generate a multitone waveform based on the updated values: **Apply Multitone**

Storing a Multitone Waveform

In this example, you learn how to store a multitone waveform. If you have not created a multitone waveform, complete the steps in the previous section, [Creating a Custom Multitone Waveform](#) on page 213.

1. Press **Load/Store > Store To File**.

If there is already a file name from the Catalog of MTONE Files occupying the active entry area, press the following keys (see [page 27](#)):

Edit Keys > Clear Text

2. Enter a file name (for example, 5TONE) using the alpha keys and the numeric keypad with a maximum length of 23 characters (see [page 27](#)).
3. Press **Enter**.

The multitone waveform is now stored in the Catalog of MTONE Files.

NOTE The RF output amplitude, frequency, and operating state settings are not stored as part of a multitone waveform file. Similarly, the multitone settings are not stored as part of the instrument state. Therefore, in most cases you should save both the instrument states and the multitone settings to be able to restore all of your settings later.

Recalling a Multitone Waveform

Using this procedure, you learn how to recall a multitone waveform from the signal generator's memory catalog.

If you have not created and stored a multitone waveform, complete the steps in the previous sections, [Creating a Custom Multitone Waveform](#) on page 213 and [Storing a Multitone Waveform](#) on page 222, then preset the signal generator to clear the stored multitone waveform from volatile ARB memory.

1. Press **Mode > Multitone**.
2. Press **Load/Store**.
3. Highlight the desired file (for example, 5TONE).
4. Press **Load From Selected File > Confirm Load From File**.
5. Press **Multitone Off On** until On is highlighted.

The firmware generates the multitone waveform in ARB memory. After waveform generation, the multitone waveform is available to be modulated on the RF output.

For instruction on configuring the RF output, see [Configuring the RF Output](#) on page 222.

13 Working in a Secure Environment

- [Understanding Memory Types](#) on page 226
- [Removing Data from Memory \(Option 006 Only\)](#) on page 228
- [Using the Secure Display \(Option 006 Only\)](#) on page 231

Understanding Memory Types

The signal generator has several memory types, and each is used to store a specific type of data. Before removing sensitive data, you should understand how each memory type is used. The following tables describe each memory type used in the base instrument, and optional baseband generator.

Table 13-1 Base Instrument Memory

Memory Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks
Main Memory (RAM) 32 MB	Yes	No	firmware operating memory no user data	operating system	CPU board, not battery backed.
Main Memory (Flash) 8 MB	Yes	Yes	factory calibration/configuration data ^a user file system, which includes flatness calibration, instrument states, and sweep lists	firmware upgrades and user-saved data ^a	CPU board (same chip as firmware memory, but managed separately) Because this memory chip contains 8 MB of user data (described here) and 8 MB of firmware memory, a full-chip erase is not desirable. User data areas are selectively and completely sanitized when you perform the Erase and Sanitize function.
Firmware Memory (Flash) 8 MB	No	Yes	main firmware image	factory installed or firmware upgrade	CPU board (same chip as main flash memory, but managed separately) During normal operation, this memory cannot be overwritten. It is only overwritten during the firmware installation or upgrade process. Because this memory chip contains 8 MB of user data and 8 MB of firmware memory (described here), a full-chip erase is not desirable. User data areas are selectively and completely sanitized when you perform the Erase and Sanitize function.
Bootrom Memory (EEPROM) 8 kB	No	Yes	CPU bootup parameters no user data	factory programmed	CPU board During normal operation, this memory cannot be overwritten or erased except for LAN configuration. This read-only data is programmed at the factory.
	Yes	Yes	LAN configuration	Front panel entry or remotely	
Calibration Data (Flash) 256 kB	No	Yes	factory calibration/configuration data backup no user data	factory or service only	RF Board

Table 13-1 Base Instrument Memory (Continued)

Memory Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Location in Instrument and Remarks
LCD Display Memory (RAM) 160 kB	No	No	display buffer	operating system	RF board, not battery backed.
Front Panel Memory (Flash) 32 kB	No	No	front panel keyboard controller firmware no user data	operating system	Front Panel board

^aAnalog instruments only


Table 13-2 Baseband Generator Memory (Options 651,652, 654)

Memory Type and Size	Writable During Normal Operation?	Data Retained When Powered Off?	Purpose/Contents	Data Input Method	Remarks
Waveform Memory (RAM) ≤ 320 MB	Yes	No	waveforms (including header and marker data)	normal user operation	Not battery backed.
Persistent Memory (Flash) 512 MB	Yes	Yes	all user data	normal user operation	User data is completely sanitized when you perform the Erase and Sanitize function.
Calibration Data Memory (Flash) 128 kB	No	Yes	no user data	factory or service only	

Removing Data from Memory (Option 006 Only)

When moving the signal generator from a secure development environment, there are several security functions you can use to remove classified proprietary information from the instrument. Security functions also have equivalent SCPI commands for remote operation (“System Subsystem (:SYSTem)” commands; refer to the *SCPI Command Reference*)

CAUTION The signal generator has several memory types (described in [Table 13-1 on page 226](#), and [Table 13-2 on page 227](#)), and each is used to store a specific type of data. Before removing sensitive data, understand how each memory type is used.

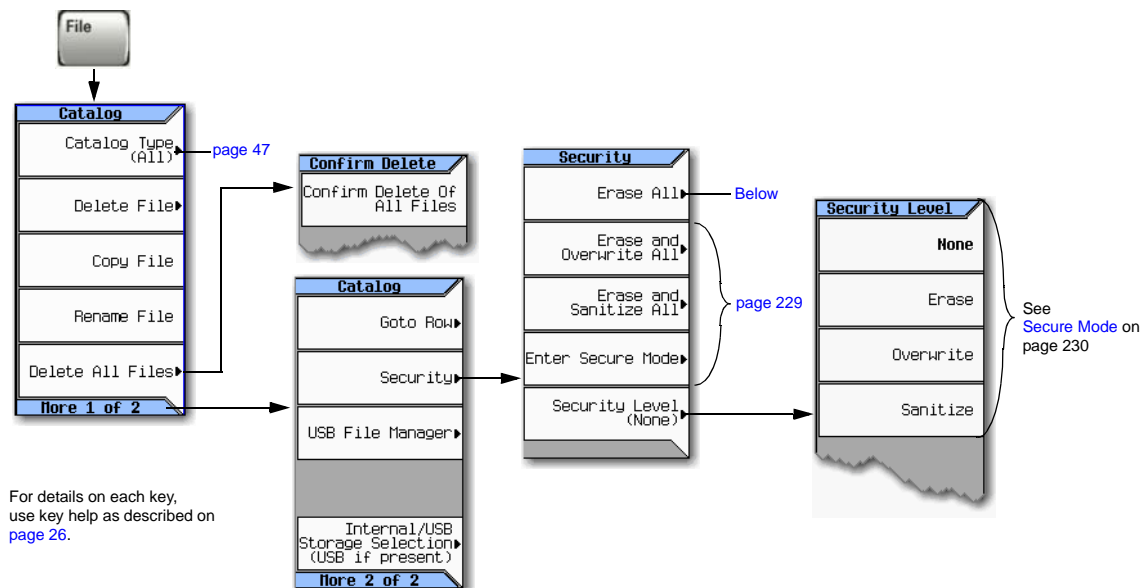

Erase All

- Removes: All user files, user flatness calibrations, user I/Q calibrations
- Resets: All table editors with original factory values, ensuring that user data and configurations are not accessible or viewable
- Does Not: Sanitize memory
- Time to Erase: typically < 1 minute, depending on the number of files.
- To Start: Press **File > More > Security > Erase All > Confirm Erase**

NOTE This is not **File > Delete All Files**, which deletes all user files but does not reset table editors.

Erase and Overwrite All

This performs the same actions as Erase All, plus it clears and overwrites the various memory types in compliance with the National Industry Security Program Operating Manual (NISPOM) DOD 5220.22M.

CPU Flash Overwrites all addressable locations with random characters and then erases the flash blocks. This accomplishes the same purpose as a chip erase. System files are restored after erase.

To Start: Press **File > More > Security > Erase and Overwrite All > Confirm Erase**

Erase and Sanitize All

This performs the same actions as Erase and Overwrite All and then adds more overwriting actions. After executing this function, you must manually perform the additional steps described below for the sanitization to comply with the National Industry Security Program Operating Manual (NISPOM) DOD 5220.22M.

CPU Flash Overwrites all addressable locations with random characters and then erases the flash blocks. This accomplishes the same purpose as a chip erase. System files are restored after erase.

BBG Persistent Memory (Flash) (*Vector instruments only*) Overwrites all addressable locations with random characters and then erases the flash blocks. This accomplishes the same purpose as a chip erase. System files are restored after erase.

To Start: Press **File > More > Security > Erase and Sanitize All > Confirm Sanitize**

Removing Persistent State Information Not Removed During Erase

Persistent State

The persistent state settings contain instrument setup information that can be toggled within predefined limits such as display intensity, contrast and the GPIB address. In vector models, the user IQ cal is also saved in this area.

The following key presses or SCPI commands can be used to clear the IQ cal file and to set the operating states that are not affected by a signal generator power-on, preset, or *RST command to their factory default:

Instrument Setup

- On the Agilent MXG front panel, press: **Utility > Power On/Preset > Restore System Settings to Default Values > Confirm Restore Sys Settings to Default Values**
- Or send this command to the Agilent MXG: `:SYSTEM:PRESet:PERSistent`

LAN Setup

The LAN setup (hostname, IP address, subnet mask, and default gateway) information is not defaulted with a signal generator power-on or *RST command. This information can only be changed

or cleared by entering new data.

User IQ Cal File (Vector Models Only)

When a user-defined IQ calibration has been performed, the cal file data is removed by setting the cal file to default, as follows:

- On the front panel, press: **I/Q** > **I/Q Calibration** > **Revert to Default Cal Settings**
- Or send this command to the Agilent MXG: `:CAL:IQ:DEF`

Secure Mode

CAUTION Once you activate secure mode (by pressing **Confirm**), you cannot deactivate or decrease the security level; the erasure actions for that security level execute at the next power cycle. Once you activate secure mode, you can only increase the security level until you cycle power. For example, you can change **Erase** to **Overwrite**, but not the reverse.

After the power cycle, the security level selection remains the same, but secure mode is not activated.

Secure mode automatically applies the selected **Security Level** action the next time the instrument's power cycles.

To Set the Level: Press **File** > **More** > **Security** > **Security Level** and choose from the following:

- **None** = factory preset, no user information is lost
- **Erase** = Erase All
- **Overwrite** = Erase and Overwrite All
- **Sanitize** = Erase and Sanitize All

To Activate: Press **File** > **More** > **Security** > **Enter Secure Mode** > **Confirm**

The softkey changes to **Secure Mode Activated**.

Securing a Nonfunctioning Instrument

If the instrument is not functioning and you are unable to use the security functions, you must physically remove the processor board and, for vector instruments, the A4 Memory Chip from the instrument. Once these assemblies are removed, choose one of the following options:

- Discard the board (or boards) and send the instrument to a repair facility. A new board (or boards) will be installed and the instrument will be repaired and calibrated. If the instrument is still under warranty, you will not be charged for new boards.
- If you have another working instrument, install the board (or boards) into that instrument and erase the memory. Then reinstall the board (or boards) back into the nonworking instrument and send it to a repair facility for repair and calibration. If you discover that one or both of the boards do not function in the working instrument, discard the nonfunctioning board and note on the repair order that it caused the instrument failure. If the instrument is still under warranty, you will not be charged for new boards.


For instructions on how to remove and replace boards, refer to the *Service Guide*.

Using the Secure Display (Option 006 Only)

This function prevents unauthorized personnel from reading the instrument display and tampering with the current configuration through the front panel. The display blanks, except for the message shown in the following figure, and the front panel keys are disabled.

To re-enable the display and front panel keys, cycle the power.

Figure 13-1 Secure Display Softkeys

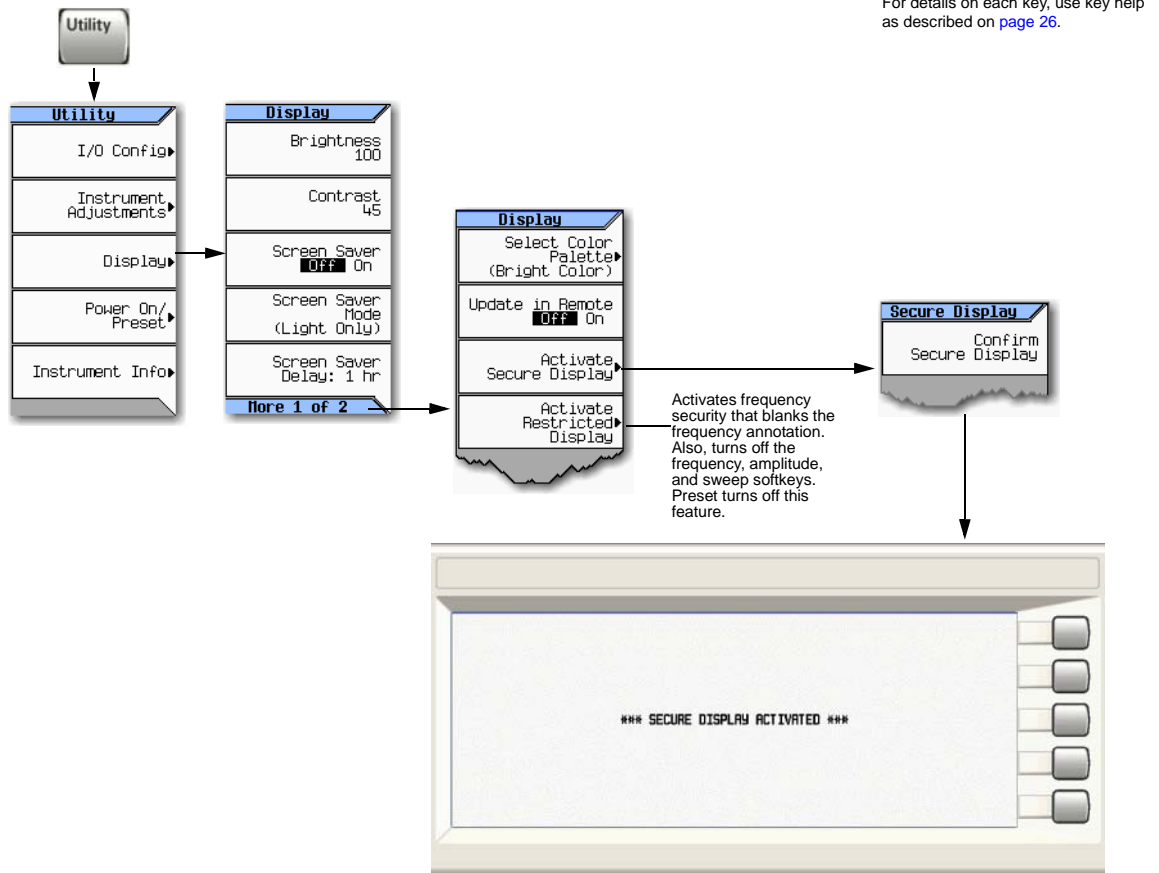

Working in a Secure Environment
Using the Secure Display (Option 006 Only)

14 Troubleshooting

- [Display](#) on page 234
- [Signal Generator Lock-Up](#) on page 234
- [RF Output](#) on page 235
 - No RF Output
 - Power Supply Shuts Down
 - No Modulation at the RF Output
 - RF Output Power too Low
 - Distortion
 - Signal Loss While Working with a Spectrum Analyzer
 - Signal Loss While Working with a Mixer on page 236
- [Sweep](#) on page 238
 - Cannot Turn Off Sweep
 - Sweep Appears Stalled
 - Incorrect List Sweep Dwell Time
 - List Sweep Information is Missing from a Recalled Register
 - Amplitude Does Not Change in List or Step Sweep on page 238
- [Internal Media Data Storage](#) on page 239
 - Instrument State Saved but the Register is Empty or Contains the Wrong State
- [USB Media Data Storage](#) on page 239
 - Instrument Recognizes USB Media Connection, but Does Not Display Files
- [Preset](#) on page 239
 - The Signal Generator Does Not Respond
 - Pressing Preset Performs a User Preset
- [Error Messages](#) on page 240
- [Front Panel Tests](#) on page 241
- [Self Test](#) on page 241
- [Licenses](#) on page 242
- [Contacting Agilent Technologies](#) on page 243
 - Returning a Signal Generator to Agilent

Display

The Display is Too Dark to Read

Both brightness and contrast may be set to minimum. Use the figure in [“Display Settings” on page 18](#) to locate the brightness and contrast softkeys and adjust their values so that you can see the display.

The Display Turns Black when Using USB Media

Removing the USB media when the instrument begins to use it can cause the screen to go black. Cycle instrument power.

Signal Generator Lock-Up

- Ensure that the signal generator is not in remote mode (the R annunciator shows on the display). To exit remote mode and unlock the front panel, press **Local Cancel/(Esc)**.
- Ensure that the signal generator is not in local lockout, which prevents front panel operation. For information on local lockout, refer to the *Programming Guide*.
- If a progress bar appears on the signal generator display, an operation is in progress.
- Preset the signal generator.
- Cycle power on the signal generator.

RF Output

No RF Output

- Check the RF ON/OFF LED (shown on [page 4](#)). If it is off, press RF On/Off to turn the output on.
- Ensure that the amplitude is set within the signal generator's range.
- If the instrument is playing a waveform, ensure that marker polarity and routing settings are correct (see [“Saving Marker Polarity and Routing Settings” on page 111](#)).

Power Supply Shuts Down

If the power supply does not work, it requires repair or replacement. If you are unable to service the instrument, send the signal generator to an Agilent service center for repair (see [page 243](#)).

No Modulation at the RF Output

Check both the Mod On/Off LED and the *<modulation>* Off On softkey, and ensure that both are on. See also, [page 43](#).

For digital modulation on a vector signal generator, ensure that the internal I/Q modulator is on (the I/Q annunciator displays).

If using an external modulation source, ensure that the external source is on and that it is operating within the signal generator's specified limits.

RF Output Power too Low

- If the AMPLITUDE area of the display shows the OFFS indicator, eliminate the offset:
Press **Amptd** > **More 1 of 2** > **Amptd Offset** > **0** > **dB**. See also, [“Setting an Output Offset” on page 75](#).
- If the AMPLITUDE area of the display shows the REF indicator, turn off the reference mode:
 1. Press **Amptd** > **More** > **Amptd Ref Off On** until *Off* highlights.
 2. Reset the output power to the desired level.See also, [“Setting an Output Reference” on page 76](#).
- If you are using the signal generator with an external mixer, see [page 236](#).
- If you are using the signal generator with a spectrum analyzer, see [page 236](#).
- If pulse modulation is on, turn off the ALC, and check that pulse width is within specifications.

Distortion

If you edit and resave a segment in a waveform sequence, the sequence does not automatically update the RMS value stored in its header. This can cause distortion on the output signal. Display the sequence header information and recalculate the RMS value (see [page 105](#)).

Signal Loss While Working with a Spectrum Analyzer

The effects of reverse power can cause problems with the RF output when you use the signal generator with a spectrum analyzer that does not have preselection. Use an unlevelled operating mode (described on [page 73](#)).

A spectrum analyzer can have as much as +5 dBm LO feedthrough at its RF input port at some frequencies. If the frequency difference between the LO feedthrough and the RF carrier is less than the ALC bandwidth, the LO's reverse power can amplitude modulate the signal generator's RF output. The rate of the undesired AM equals the difference in frequency between the spectrum analyzer's LO feedthrough and the signal generator's RF carrier.

Reverse power problems can be solved by using one of the unlevelled operating modes.

See:

- “ALC Off Mode” on [page 74](#)
and
- “Power Search Mode” on [page 74](#)


Signal Loss While Working with a Mixer

To fix signal loss at the signal generator's RF output during low-amplitude coupled operation with a mixer, add attenuation and increase the RF output amplitude.

The figure at right shows a configuration in which the signal generator provides a low amplitude signal to a mixer.


The internally leveled signal generator RF output (and ALC level) is -8 dBm. The mixer is driven with an LO of +10 dBm and has an LO-to-RF isolation of 15 dB. The resulting -5 dBm LO feedthrough enters the signal generator's RF output connector and arrives at the internal detector.

Depending on frequency, it is possible for most of this LO feedthrough energy to enter the detector. Because the detector responds to its total input power regardless of frequency, this excess energy causes the ALC to reduce the RF output. In this example, the reverse power across the detector is actually greater than the ALC level, which can result in loss of signal at the RF output.

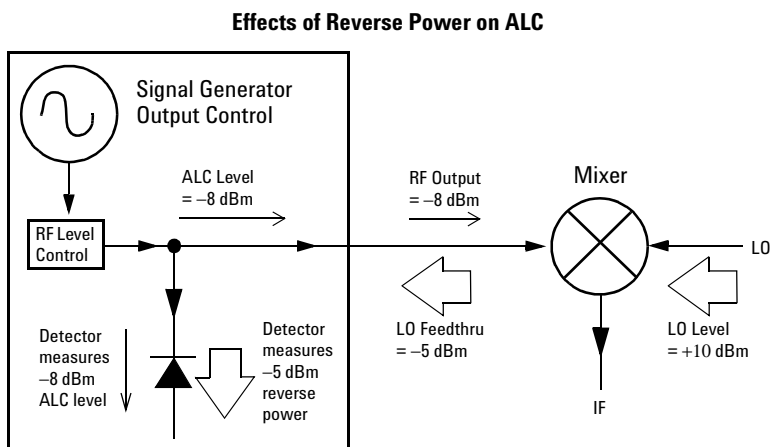

The solution at right shows a similar configuration with the addition of a 10 dB attenuator connected between the RF output of the signal generator and the input of the mixer. The signal generator's ALC level increases to +2 dBm and transmits through a 10 dB attenuator to achieve the required -8 dBm amplitude at the mixer input.

Compared to the original configuration, the ALC level is 10 dB higher while the attenuator reduces the LO feedthrough (and the signal generator's RF output) by 10 dB. Using the attenuated configuration, the detector is exposed to a +2 dBm desired signal versus the -15 dBm undesired LO feedthrough. This 17 dB difference between desired and undesired energy results in a maximum 0.1 dB shift in the signal generator's RF output level.

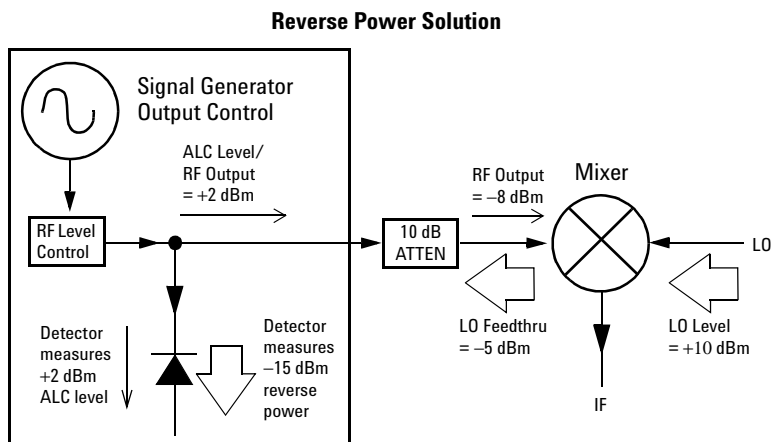

Sweep

Cannot Turn Off Sweep

Press **Sweep > Sweep > Off**.

Sweep Appears Stalled

The current status of the sweep is indicated as a shaded rectangle in the progress bar (see [“Configuring a Swept Output” on page 31](#)). If the sweep appears to stall, check the following:

1. Turn on the sweep with one of the following key sequences:
 - Sweep > Sweep > Freq**
 - Sweep > Sweep > Amptd**
 - Sweep > Sweep > Waveform** (vector instruments only)
2. If the sweep is in single mode, press the **Single Sweep** softkey.
3. If the sweep trigger (indicated by the **Sweep Trigger** softkey) is *not* set to Free Run, set it to Free Run to determine if a missing sweep trigger is blocking the sweep.
4. If the point trigger (indicated by the **Point Trigger** softkey) is *not* set to Free Run, set it to Free Run to determine if a missing point trigger is blocking the sweep.
5. Set the dwell time to one second to determine if the dwell time was set to a value that was too slow or too fast to see.
6. Ensure that you set at least two points in the step sweep or list sweep.

Incorrect List Sweep Dwell Time

1. Press **Sweep > More > Configure List Sweep**.
2. Check that the list sweep dwell values are accurate.
3. If the dwell values are incorrect, edit them.
If the dwell values are correct, continue to the next step.
4. Press **More**, and ensure that the **Dwell Type List Step** softkey is set to List.
If Step is selected, the signal generator sweeps the list points using the dwell time set for step sweep rather than list sweep.

See also, [“Configuring a Swept Output” on page 31](#).

List Sweep Information is Missing from a Recalled Register

List sweep information is not stored as part of the instrument state in an instrument state register. Only the current list sweep is available to the signal generator. You can store list sweep data in the instrument catalog (see [“Loading \(Recalling\) a Stored File” on page 49](#)).

Amplitude Does Not Change in List or Step Sweep

Verify that sweep type is set to amplitude (Amptd); the amplitude does not change when the sweep type is set to frequency (Freq) or waveform.

Internal Media Data Storage

Instrument State Saved but the Register is Empty or Contains the Wrong State

If the register number you intended to use is empty or contains the wrong instrument state, recall register 99. If you selected a register number greater than 99, the signal generator automatically saves the instrument state in register 99.

See also, [“Working with Instrument State Files” on page 51](#).

USB Media Data Storage

Instrument Recognizes USB Media Connection, but Does Not Display Files

If the USB media works on other instruments or computers, it may simply be incompatible with the signal generator; try a different USB media. Refer to <http://www.agilent.com/find/mxg> for details on compatible USB media.

Preset

The Signal Generator Does Not Respond

If the signal generator does not respond to a preset, the instrument may be in remote mode, which locks the keypad.

To exit remote mode and unlock the preset keys, press **Local Cancel/(Esc)**.

Pressing Preset Performs a User Preset

This behavior results from the use of a backward-compatible SCPI command. To return the signal generator to normal use, send the command `:SYST:PRESet:TYPE NORM`.

For information on SCPI commands, refer to the *SCPI Command Reference*.

Error Messages

Error Message Types

Events do not generate more than one type of error. For example, an event that generates a query error does not generate a device-specific, execution, or command error.

Query Errors (-499 to -400) indicate that the instrument's output queue control has detected a problem with the message exchange protocol described in IEEE 488.2, Chapter 6. Errors in this class set the query error bit (bit 2) in the event status register (IEEE 488.2, section 11.5.1). These errors correspond to message exchange protocol errors described in IEEE 488.2, 6.5. In this case:

- Either an attempt is being made to read data from the output queue when no output is either present or pending, or
- data in the output queue has been lost.

Device Specific Errors (-399 to -300, 201 to 703, and 800 to 810) indicate that a device operation did not properly complete, possibly due to an abnormal hardware or firmware condition. These codes are also used for self-test response errors. Errors in this class set the device-specific error bit (bit 3) in the event status register (IEEE 488.2, section 11.5.1).

The <error_message> string for a *positive* error is not defined by SCPI. A positive error indicates that the instrument detected an error within the GPIB system, within the instrument's firmware or hardware, during the transfer of block data, or during calibration.

Execution Errors (-299 to -200) indicate that an error has been detected by the instrument's execution control block. Errors in this class set the execution error bit (bit 4) in the event status register (IEEE 488.2, section 11.5.1). In this case:

- Either a <PROGRAM DATA> element following a header was evaluated by the device as outside of its legal input range or is otherwise inconsistent with the device's capabilities, or
- a valid program message could not be properly executed due to some device condition.

Execution errors are reported *after* rounding and expression evaluation operations are completed. Rounding a numeric data element, for example, is not reported as an execution error.


Command Errors (-199 to -100) indicate that the instrument's parser detected an IEEE 488.2 syntax error. Errors in this class set the command error bit (bit 5) in the event status register (IEEE 488.2, section 11.5.1). In this case:

- Either an IEEE 488.2 syntax error has been detected by the parser (a control-to-device message was received that is in violation of the IEEE 488.2 standard. Possible violations include a data element that violates device listening formats or whose type is unacceptable to the device.), or
- an unrecognized header was received. These include incorrect device-specific headers and incorrect or unimplemented IEEE 488.2 common commands.

Error Message File

A complete list of error messages is provided on the CDROM supplied with the instrument. In the error message file, an explanation is generally included with each error to further clarify its meaning. The error messages are listed numerically. In cases where there are multiple listings for the same error number, the messages are in alphabetical order.


Front Panel Tests

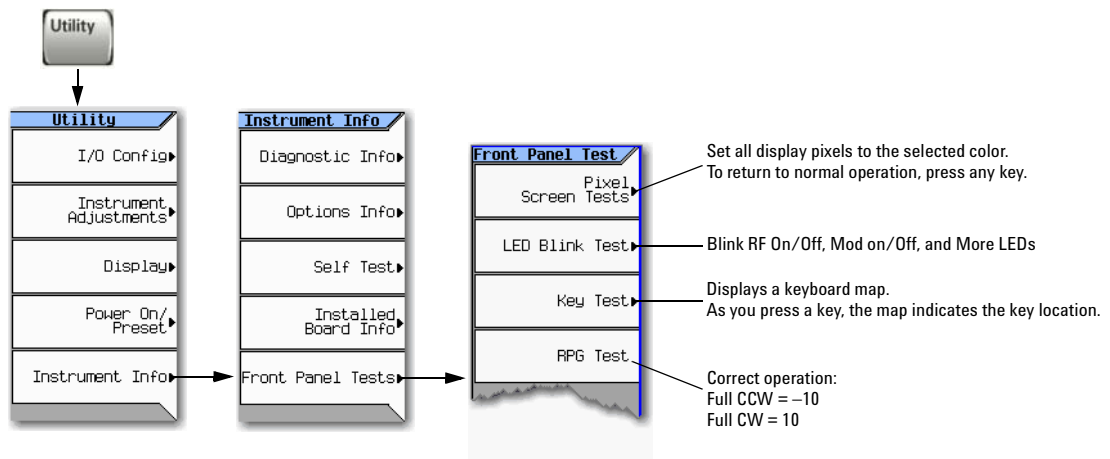

For details on each key, use key help as described on [page 26](#).

Self Test

The self test is a series of internal tests that checks different signal generator functions.

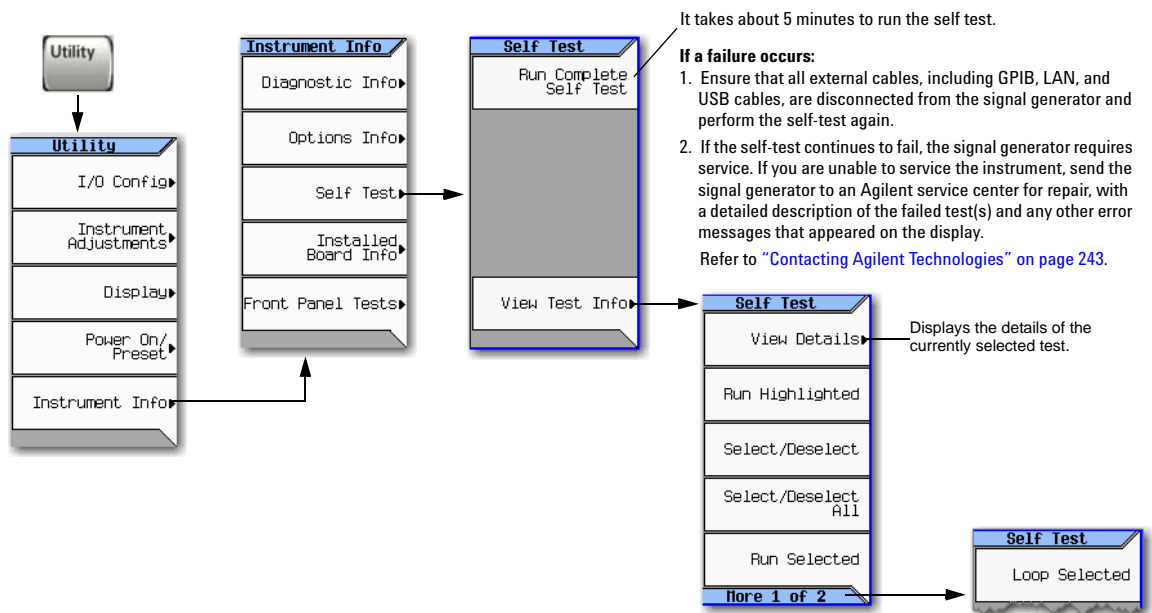

Licenses

A Time-Based License Quits Working

- The instrument's time or date may have been reset forward causing the time-based license to expire.
- The instrument's time or date may have been reset backward more than approximately 25 hours, causing the instrument to ignore time-based licenses.

See [page 20](#) for details and cautions on setting time and date.

Cannot Load a Time-Based License

The instrument's time or date may have been reset backward more than approximately 25 hours, causing the instrument to ignore time-based licenses.

See [page 20](#) for details and cautions on setting time and date.

Contacting Agilent Technologies

- assistance with test and measurements needs, and information on finding a local Agilent office: <http://www.agilent.com/find/assist>
- accessories or documentation: <http://www.agilent.com/find/mxg>
- new firmware releases: <http://www.agilent.com/find/upgradeassistant>.

If you do not have access to the Internet, please contact your field engineer.

NOTE In any correspondence or telephone conversation, refer to the signal generator by its model number and full serial number. With this information, the Agilent representative can determine whether your unit is still within its warranty period.

Returning a Signal Generator to Agilent

Use the following steps to return a signal generator to Agilent Technologies for servicing:

1. Gather as much information as possible regarding the signal generator's problem.
2. Call the phone number listed on the Internet (<http://www.agilent.com/find/assist>) that is specific to your geographic location. If you do not have access to the Internet, contact your Agilent field engineer.

After sharing information regarding the signal generator and its condition, you will receive information regarding where to ship your signal generator for repair.

3. Ship the signal generator in the original factory packaging materials, if available, or use similar packaging to properly protect the signal generator.

Glossary

A

Active Entry The currently selected, and therefore editable, entry or parameter

ARB Arbitrary waveform generator

AWG Arbitrary waveform generator. Additive white Gaussian noise

B

BBG Media Baseband generator media. Volatile memory, where waveform files are played or edited.

BNC Connector Bayonet Neill-Concelman connector. A type of RF connector used to terminate coaxial cable.

C

CCW Counterclockwise

C/N Carrier-to-noise ratio

CW Continuous wave. Clockwise

D

DHCP Dynamic host communication protocol

Dwell Time In a step sweep (see [page 33](#)), the time that the signal is settled and you can make a measurement before the sweep moves to the next point.

E

EVM Error vector magnitude; the magnitude of the vector difference at a given instant between the ideal reference signal and the measured signal.

F

Filter factor Alpha The filter's alpha coefficient. It is only valid for root nyquist and nyquist filters.

Filter Factor BbT The filter's bandwidth-bit-time (BbT). It is only valid for a Gaussian filter (similar to alpha). BbT is defined by the GSM standard as 0.3 and by the DECT standard as 0.5.

G

Gaussian filter The Gaussian filter does not have a zero Inter-Symbol Interference (ISI). Wireless system architects must decide just how much of the ISI can be tolerated in a system and combine that with noise and interference. The Gaussian filter is gaussian shaped in both the time and frequency domains, and it does not ring like the root nyquist filters do. The effects of this filter in the time domain are relatively short and each symbol interacts significantly (or causes ISI) with only the preceding and succeeding symbols. This reduces the tendency for particular sequences of symbols to interact, which makes amplifiers easier to build and more efficient.

GPIB General purpose interface bus. An 8-bit parallel bus common on test equipment.

H

Hardkey A labeled button on the instrument.

I

IF Intermediate frequency

Int Media Internal media. Non-volatile signal generator memory, where waveform files are stored.

IP Internet protocol. The network layer for the TCP/IP protocol suite widely used on Ethernet

networks.

L

LAN Local area network

LO Local oscillator

LXI LAN extension for instrumentation. An instrumentation platform based on industry standard Ethernet technology designed to provide modularity, flexibility, and performance to small- and medium-sized systems. See also, <http://www.lxistandard.org>

M

Modulation Format Custom modulation, Two Tone, or Multitone.

Modulation Mode Dual ARB, Custom modulation, Two Tone, or Multitone.

Modulation Standard Refers to a Cellular standard format (i.e. NADC, PDC, PHS, etc.).

Modulation Type Refers to the various I/Q constellation types (i.e. PSK, MSK, FSK, C4FM, etc.)

N

Non-volatile That which survives a power cycle (such as files stored in USB media).

Nyquist filter Also referred to as a cosine filter. These filters have the property that their impulse response rings at the symbol rate. Adjacent symbols do not interfere with each other at the symbol times because the response equals zero at all symbol times except the center (desired) one.

P

Persistent That which is unaffected by preset, user preset, or power cycle.

Point-to-point Time In a step sweep (page 33), the sum of the dwell time, processing time, switching time, and settling time.

R

Rectangular filter Also referred to as a ideal low pass filter. These filters have very steep cut-off characteristics. The pass band is set to equal the symbol rate of the signal. Due to a finite number of coefficients, the filter has a predefined length and is not truly “ideal”. The resulting ripple in the cut-off band is effectively minimized with a Hamming window. This filter is recommended for achieving optimal ACP. A symbol length of 32 or greater is recommended for this filter.

Root Nyquist filter Also referred to as a Root cosine filter. These filters have the property that their impulse response rings at the symbol rate. Adjacent symbols do not interfere with each other at the symbol times because the response equals zero at all symbol times except the center (desired) one. Root nyquist filters heavily filter the signal without blurring the symbols together at the symbol times. This is important for transmitting information without errors caused by ISI. Note that ISI does exist at all times except the symbol (decision) times. A cascade of two of these filters has the transfer function of a Nyquist filter. One is in the transmitter, the other in the receiver, so that the system taken as a whole has the zero-ISI properties of an ISI filter.

RMS Root mean square. A time-varying signal's effective value (the equivalent DC voltage required to generate the equivalent heat across a given resistor). For a sinewave, $RMS = 0.707 \times$ peak value.

S

Softkey A button located along the instrument's display that performs whatever function is shown next to it on that display.

T

TCP Transmission control protocol. The most common transport layer protocol used on Ethernet and the Internet.

Terminator A unit indicator (such as Hz or dBm) that completes an entry. For example, for the entry 100 Hz, *Hz* is the terminator.

Type-N Connector Threaded RF connector used to join coaxial cables.

U

USB Universal serial bus. See also, <http://www.usb.org>

User FIR Selects a user-defined set of coefficient values. Each line in the FIR values table contains one coefficient value. The number of coefficient values listed must be a multiple of the selected oversampling ratio. Each coefficient applies to both I and Q components.

V

Volatile That which does not survive a power cycle (such as files stored in BBG media).

Symbols**ΦM**

- annunciator 9
- dc offset, removing 83
- hardkey 81
- softkeys 81, 83
- # points softkey 33
- # Skipped Points softkey 115

Numerics

- 10 MHz OUT connector 13
- 100Base-T LAN cable 22
- 1410, application note 214
- 430, option
 - multitone mode 220
 - two-tone 214
 - two-tone mode 214
- 5-Pack
 - history, waveform files 171
 - licensing 164
 - licensing, installing 165
 - licensing, understanding 164
 - licensing, waveform file 165
 - status messages 167
 - warning messages 175
- 628, error 149
- 651/652/654, option
 - description 3
 - multitone mode 220
 - two-tone mode 214
- 670/671/672, option
 - description 3
- 8557D GPIB only softkey 23
- 8648A/B/C/D GPIB only softkey 23
- 8656B,8657A/B GPIB only softkey 23

A

- AC power receptacle 11
- ACP 190
- Activate Secure Display softkey 18
- active
 - entry 245
 - entry area 8
- Active High softkey 127
- Active Low softkey 127
- Add Comment To softkey 51
- additive white Gaussian noise. *See* AWGN
- address, GPIB 21
- Adjust Phase softkey 29
- Adjustable doublet softkey 86
- adjustments
 - I/Q 92, 155
 - quadrature 155
 - real-time phase noise 187
- advance, segment 129

- Advanced Settings softkey 22
- Aeroflex softkey 23
- Agilent MXG
 - modes of operation 3
- Agilent sales and service offices 243
- ALC
 - hold 111, 112
 - OFF annunciator 9
 - off mode 74
 - softkeys 29, 115
- All softkey 46
- Alpha 245
- AM
 - annunciator 9
 - connector 12
 - external source 83
 - hardkey 81
 - softkeys 81
- amplitude
 - display area 10
 - hardkey 29
 - modulation 81
 - offset 75
 - reference 76
 - setting 29
 - softkeys 29–38
 - troubleshooting sweep 238
- AMPTD hardkey 29
- Amptd softkeys 29–38
- analog modulation 3, 81
- angle, quadrature 92
- annunciators 9
- APCO 25 w/C4FM softkey 192
- APCO 25 w/CQPSK softkey 192
- apodization settings, FIR filter 209
- application notes
 - 1410 214
- Apply To Waveform softkey 115
- ARB
 - definition 245
 - player, dual 96
 - softkeys 96, 125, 179, 184
 - waveform clipping 133
- arb 190
- Arb Segment softkey 50
- Arb Sequence softkey 50
- ARMED annunciator 9
- arrow keys 27
- ATTEN HOLD annunciator 9
- Atten/ALC Control softkey 29
- Auto softkeys
 - (DHCP/Auto-IP) 22
 - Auto 73
 - Recall 80
- AUTOGEN_WAVEFORM file 190

Index

auto-IP 22
Auto-IP softkey 22
Automatically Use USB Media If Present softkey 46
AUX I/O connector 15
Auxiliary Software Options softkey 24
AWGN
 adding 177
 annunciator 9
 definition 245
 dual ARB player 178
 softkeys 181
AWGN softkeys 179

B

backspace hardkey 27
Bandwidth softkey 181
baseband 15
 aligning signals at 111
 clipping 133
 frequency offset
 softkey location 149
 frequency offset, setting 149
 I/Q output connectors 14
 memory 96, 226
 noise 177
 noise annunciator 9
 quadrature adjustment 155
 real time I/Q AWGN 179, 181
 softkey 149
 summing signals 154
 waveforms convert to analog 144
baseband frequency offset
 DAC over range & scaling 150
 softkey 149
baseband generator 190
 custom arb mode 3
 dual arb mode 3
 multiple BBG synchronization 158
 multitone mode 3, 220
 two-tone mode 214
BB GEN 154
BBG
 media 96, 98
 media (definition) 245
 Memory softkey 50
 Memory to USB softkey 50
 routing 154
 Segments softkey 46, 105
BBG sync 158
 configure setup 161
 equipment setup 161
 resynchronization 163
 system 160
 system delay 160
 trigger setup 160

BbT 245
Binary softkey 46
Bk Sp hardkey 27
Bluetooth softkey 192
BNC 245
bootrom memory 226
Bright Color softkey 18
brightness adjustment 18
Brightness softkey 18
Buffered Trig softkey 127
Build New Waveform Sequence softkey 101, 123
Burst Envelope softkey 152
Bus softkey 31

C

C/N 245
cables
 crossover 22
 multi-BBG sync 160
cables, 100Base-T LAN 22
Calculate softkey 105
calibration
 data 226
 data memory 227
 I/Q 157
 softkey 157
Calibration Type softkey 157
Cancel hardkey 5
carrier
 bandwidth 178
 configuring 29
 feedthrough 92
 modulating 43
 softkeys 179
 to noise ratio 178
Carrier Bandwidth softkey 179
carrier feedthrough, minimizing 217
Carrier to Noise softkey 179
Catalog Type softkey 46, 47, 50, 105
catalog, state files 54
ccw 245
CDPD softkey 192
Channel Band softkey 29
Channel Number softkey 29
circular clipping 137, 140
classified. *See* security
Clear softkeys
 Error Queue(s) 56
 Header 105
 Text 27
clipping
 circular 137, 140
 rectangular 138, 141
 softkeys 133
clock, sample rate 15

- coefficient values, entering 205
- color palette, display 18
- comments, adding & editing (instrument state) 52
- component test 190
- Config Type softkey 22
- Configure softkeys
 - Cal Array 59
 - List Sweep 31, 38
 - Step Array 59
 - Step Sweep 31, 33
- Confirm Load From File softkey 49
- Connection Monitoring softkey 22
- Connection Type softkeys
 - Sockets 62
 - USB 62
 - VXI-11 62
- connectors
 - external triggering source 130, 132
 - front panel 4
 - rear panel 11
 - routing signals 32
- Continuous softkey 127
- continuous step sweep example 41
- continuous wave
 - description 3
- continuous wave output 29
- contrast adjustment 18
- Contrast softkey 18
- Copy & softkeys
 - Play Sequence 49
 - Play Waveform 49
 - Select User Flatness 49
 - Select User Flatness Corrections 49
- Copy softkeys
 - All Files 50
 - File 46
 - File to Instrument 46, 50
 - File to USB 50
- correction array (user flatness) 64
 - viewing 65
 - See also* user flatness correction
- cosine filter. *See* nyquist filter
- Create Directory softkey 46, 50
- crossover cable 22
- custom
 - multicarrier TDMA waveforms
 - creating 201
 - TDMA digital modulation 195
- Custom ARB softkeys 191
- custom arb waveform generator 3
- custom mode 190
- cw 245
- CW (no modulation) softkey 38
- CW mode
 - description 3

D

- D01 164
- DAC over range error 144, 149
- DAC over range protection
 - baseband frequency offset 150
 - phase noise 188
- Dark Color softkey 18
- data
 - calibration 226
 - entry softkeys 27
 - erasing 228
 - files 45–51
 - removing 228
 - serial, synchronizing 15
 - storage
 - comments, adding and editing 52
 - troubleshooting 239
 - type 55
 - using 45
- date, setting 20
- dc offset 92
- dc offset, removing 83
- DCFMΦ/DCFM Cal softkey 81
- DECT softkey 192
- Default Gateway softkey 22
- default settings
 - restoring 19, 22, 157
 - system, restoring 26
- Default softkey 192
- delay
 - I/Q 155
 - multiple BBG sync 160
- Delete softkeys
 - All Regs in Seq 51
 - All Segments On Int Media 98
 - All Segments On USB Media 98
 - All Sequence Files 46
 - All Sequences 51, 80
 - All Waveforms 101
 - All Waveforms softkey 123
 - File 46
 - File or Directory 46, 47, 50, 55
 - Item 38
 - Row 38
 - Selected Waveform 101, 123
 - Seq Reg 51
 - Waveform Sequence 123
- description & plots, phase noise 185
- DETHTR annunciator 9
- Device softkey 29
- DHCP 22, 245
- DHCP softkey 22
- Diff Mode softkeys 155
- DIGBUS annunciator 9
- digital bus 15

Index

- digital modulation
 - formats 3
 - multitone 220–223
 - TDMA 195
 - two tone 214–219
- digital operation 95, 164
- digital signal to analog waveform 144
- display
 - blanking 231
 - error message area 10
 - memory 226
 - overview 4, 8
 - secure 231
 - settings 18
 - softkey labels 10
 - softkeys 17, 27, 115
 - tests 241
 - text area 10
 - troubleshooting 234
- Display softkeys
 - Case 27
 - display 17
 - Waveform And Markers 115
- Displayed Case softkeys 27
- distortion, troubleshooting 235
- DNS Server Override softkey 22
- DNS Server softkey 22
- documentation xi
- Domain Name softkey 22
- doublet
 - adjustable 88
 - softkeys 86
 - trigger 88
- dual ARB
 - multi-BBG sync 158
 - player 96
 - real-time noise 178
 - softkeys 97, 179, 184
- dual arb 190
- dual ARB player 3
- dual arbitrary waveform generator 3
- dwelt time 38, 245
- Dwell Type softkey 38
- dwelt, troubleshooting 238
- Dynamic DNS Naming softkey 22
- Dynamic Hostname Services softkey 22

E

- E4428C, E4438C softkey 23
- E442xB, E443xB softkey 23
- E8241A, E8244A, E8251A, E8254A softkey 23
- E8247C, E8257C, E8267C softkey 23
- E8257D, E8267D softkey 23
- EDGE softkey 192
- Edit softkeys

- Description 105
- Noise RMS Override 105
- Repetitions 123
- RMS 105
- Selected Waveform Sequence 101, 123
- Editing Keys softkey 27
- Editing Mode softkey 27
- EEPROM 226
- Enable/Disable Markers softkey 101, 123
- Enter Directory softkey 49
- entry, active 245
- equipment setup 161
- equipment, user flatness correction 60, 61
- ERR annunciator 9
- Error hardkey 56
- error messages 56
 - DAC over range 144, 149
 - display area 10
 - file 240
 - message format 56
 - types 240
- Esc hardkey 5
- EVENT
 - connector, AUX I/O 15
 - connector, BNC 14, 110
 - output jitter 125
 - outputs 110
- EVM 245
- EVM error 92
- example
 - 5-Pack License, adding 168
 - 5-Pack License, history 173
 - Waveform 5-Pack License, adding 168
 - Waveform 5-Pack License, history 173
- examples
 - FIR filters
 - creating 204
 - modifying 208
- Execute Cal softkey 157
- EXT CLOCK connector 14
- EXT REF annunciator 9
- Ext softkeys
 - Delay 128
 - Delay Time 128
 - Ext 31
 - I/Q Output 152, 153
 - Pulse 86
 - Source 128
- extension, file 49
- external
 - I and Q signals 154
 - media 55, 239
 - modulation source 83
 - reference oscillator, using 30
 - trigger source 130, 132

- triggering 132
 - external leveling 67–73
 - softkeys 67
 - external leveling, configuring 70
 - External softkeys
 - External 152
 - Input 155
 - Input I Offset 92
 - Input Q Offset 92
 - Output 155
- F**
- factory defaults, restoring 19, 22, 157
 - features 2
 - feedthrough 92
 - feedthrough, carrier, minimizing 217
 - File hardkey 46, 54
 - file headers
 - creating 105
 - editing 107
 - example 107
 - viewing a different file 109
 - files
 - catalog. *See* data storage
 - extensions 49
 - working with 45
 - filter, interpolator 144
 - filters
 - gaussian, loading default 209
 - nyquist, selecting 198
 - FIR filter
 - apodization settings 209
 - Hamming 209
 - Hann 209
 - Kaiser 209
 - window settings 209
 - FIR filters
 - creating 204
 - modifying 208
 - storing 207
 - FIR table editor
 - accessing 204
 - coefficients, duplicating 206
 - coefficients, entering values 205
 - coefficients, modifying 210
 - files, loading 209
 - filters
 - creating 204
 - modifying 208
 - storing 207, 211
 - oversample ratio, setting 206
 - firmware
 - memory 226
 - upgrading 20, 243
 - First Mkr Point softkey 115
 - First Sample Point softkey 115
 - Fixed softkey 73
 - flash memory 226
 - flatness correction. *See* user flatness correction
 - Flatness softkey 59
 - FM
 - annunciator 9
 - connector 12
 - dc offset, removing 83
 - external source 83
 - hardkey 81
 - softkeys 81
 - Free Run softkey 31, 78, 127
 - Free-Run softkey 86
 - FREQ hardkey 29
 - Freq softkeys 29–38, 59
 - frequency
 - display area 8
 - hardkey 6, 7, 29
 - modulation 81
 - multiplier 77
 - offset 75
 - offset, baseband 149
 - offset, softkeys 149
 - reference 76
 - setting 29
 - softkeys 29, 29–38
 - step sweep 35
 - front panel
 - disabling keys 231
 - display 8
 - I/Q inputs, using 93
 - knob resolution 19
 - overview 4
 - tests 241
 - FTP Server softkey 22
 - fundamental operation *See* basic operation
- G**
- Gated softkey 86, 127
 - gated triggering 127, 130
 - Gaussian
 - definition 245
 - gaussian filter, loading default 209
 - Gaussian. *See* AWGN
 - glossary 245
 - Go To Default Path softkey 46, 47, 55
 - Goto Row softkey 38, 46
 - GPIO
 - connector 13
 - definition 245
 - setup 21
 - softkeys
 - Address 21
 - Setup 21

Index

green LED 7
GSM softkey 192
guides, content of xi

H

hardkeys
 definition 245
 help on 26
 overview 4
 See also specific key
header utilities softkeys 105
Help hardkey 5, 26
Hostname softkey 22
hostname, setting 22
HP 3300A, emulating 80

I

I connector 6
I Offset softkey 155
I OUT connector 14
I/O Config softkey 17
I/Q
 adjustments 92, 155
 front panel inputs, using 93, 154
 modulation 92, 152
 optimizing 153
 rear panel outputs 14
 rear panel outputs, using 153
 signal path, optimizing 153
 signal, aligning 111
 softkeys 92, 152–157
 waveform, clipping 133
ideal low-pass filter. *See* rectangular filter
IF 245
images 92
impairments
 I/Q adjustments 92
impairments, real-time
 phase noise 183
Import Waveform softkey 123
Incr Set hardkey 7
information, removing from memory 228
Insert softkeys
 Insert 101
 Item 38
 Row 38
 Waveform 101
 Waveform Sequence Contents 101
Install licenses softkey 49
installation guide content xi
instrument
 8757D Scalar Network Analyzer 36
 firmware, upgrading 20
 scalar network analyzer 36
 softkeys

 Adjustments 17
 Info 17
 Options 24
 state
 associating with waveform 52
 files 51, 54
 register. *See* data storage
 softkey 50
int media 245
Int Phase Polarity softkey 152
interface
 GPIB 21
 LAN 22
Internal Baseband Adjustments softkey 155
internal media 55
Internal Storage to USB softkey 50
Internal/USB Storage Selection softkey 46
interpolator filter 144
IP
 Address softkey 22
 address, setting 22
 auto 22
 definition 245

J

jitter on EVENT output 125

K

keyboard, using 80
keys
 disabling 231
 front panel 4
 help on 26
 numeric 4
 test 241
 See also specific key
knob 7, 19, 27

L

L annunciator 9
LAN
 connector 13
 definition 246
 Services Setup softkey 21
 setup 22
 Setup softkey 21
Last Mkr Point softkey 115
Last softkey 19
LCD display memory 226
LEDs 7
 blink test 241
 front panel 7
 modulation 43
leveling
 external 67–73

- turn off ALC 74
 - licenses
 - manager 24
 - service software 24
 - signal studio 24
 - time-based 20
 - troubleshooting 242
 - viewing 24
 - waveform 24
 - line power (green) LED 7
 - linear sweep 33
 - list mode values 39
 - List softkey 46
 - list sweep
 - parameters 39
 - status information 39
 - troubleshooting 238
 - using 38
 - waveform 40
 - listener mode annunciator 9
 - LO 246
 - Load From Selected File softkey 48, 49
 - Load List softkey 49
 - Load softkeys
 - All From Int Media 98
 - All From USB Media 98
 - Cal Array From Step Array 59
 - From Selected File 48, 49
 - Load/Store 38, 48, 49
 - Segment From Int Media 98
 - Segment From USB Media 98
 - Store 98
 - Sweep List 49
 - Load/Store softkey 38, 48, 49
 - Local hardkey 5
 - lock up, troubleshooting 234
 - logarithmic sweep 33
 - LXI 246
- M**
- main memory 226
 - manual control, sweep 42
 - Manual softkey 73
 - Manual softkeys
 - Config Settings 22
 - Manual 22
 - Mode 31
 - Point 31
 - manuals, content of xi
 - Marker softkeys 115
 - markers
 - frequency
 - N5183A 37
 - step sweep 37
 - markers, aligning signal 111
 - markers, waveform 110–125
 - media
 - BBG 245
 - erasing 228
 - int 245
 - memory stick 55
 - storage 55
 - types 96, 226
 - USB 55, 239
 - memory
 - erasing data from 228
 - types 226
 - See also* media
 - menu keys 5
 - messages, error 240
 - messages, warning
 - 5-Pack Licensing 175
 - Waveform 5-Pack Licensing 175
 - mirror table, duplicating coefficients 206
 - mixer, troubleshooting signal loss 236
 - Mod On/Off hardkey 6, 43
 - Mode hardkey 97, 179, 181, 184
 - mode, modulation 246
 - modes of operation 3
 - Modulated softkey 73
 - modulation
 - AM 81
 - analog 3
 - annunciators 9
 - carrier signal 43
 - digital 3
 - external source, using 83
 - FM 81
 - generating 43
 - I/Q 92, 152
 - phase 81
 - pulse 3, 85
 - simultaneous 44
 - troubleshooting 235
 - Modulator Atten softkey 181
 - monochrome display, setting 18
 - Monochrome softkey 18
 - MULT annunciator 9
 - multi-BBG sync 158
 - configure setup 161
 - equipment setup 161
 - resynchronize 163
 - system delay 160
 - system sync 160
 - trigger setup 160
 - multicarrier setup
 - APCO 25 w/C4FM 201
 - APCO 25 w/CQPSK 201
 - Bluetooth 201
 - CDPD 201

Index

- DECT 201
- Default 201
- EDGE 201
- GSM 201
- NADC 201
- PDC 201
- PHS 201
- PWT 201
- TETRA 201
- multicarrier setup softkeys 201
- multicarrier TDMA waveforms
 - creating 201
- multicarrier, Default softkey. *See* quick setup, Default softkey, settings
- multiplier, using 77
- multitone 190, 220–223
- multitone mode 3
- Multitone softkeys 220
- multitone waveform, setup 213

N

- N7699A-D01 164
- NADC softkey 192
- Name And Store softkey 123
- Next REG softkey 80
- Next SEQ softkey 80
- No action softkey 49
- No Retrigger softkey 127
- noise 177
- noise bandwidth factor 178
- non-volatile memory 96
- non-volatile, definition 246
- number keys 27
- numeric keypad 4
- nyquist filter
 - definition
- nyquist filter, selecting 198

O

- OFFS annunciator 9
- offset 92
- offsets
 - baseband frequency 149
 - I/Q 155
 - output, using 75
- on/off switch 7
- operation
 - modes of 3
- operation, basic 25
- operation, remote 21
- optimization, I/Q 92, 152
- option
 - 430
 - multitone mode 220
 - two tone mode 214

- two-tone mode 214
- Option 22x 164
- options
 - 651/652/654
 - description 3
 - multitone mode 220
 - two-tone mode 214
 - 670/671/672, description 3
 - enabling 17, 24
 - resource 2
 - UNT 3
 - UNU 3
 - UNW 3
- Options 221-229 164
- Options Info softkey 24
- oscillator, external reference 30
- Output Blanking softkey 29
- output, swept 31
- over range error, DAC 144, 150, 188
- overshoot 144
- overview, signal generator 1

P

- Page Up hardkey 5
- parameters, saving a waveform's 105
- path delay 92
- PATT TRIG IN connector 15
- Patt Trig In softkeys 128
- PDC softkey 192
- peak-to-average power, reducing 137
- performance, optimizing 57
- persistent
 - memory 227
- persistent settings
 - definition 246
 - resetting 26
 - restoring defaults 19
- phase noise
 - adjustments 187
 - DAC over range & scaling 188
 - description & plots 185
 - impairments 183
 - softkeys 184
- Phase Ref Set softkey 29
- phase skew 92
- PHS softkey 192
- pixel test 241
- Plot CDDF softkey 143
- PM Config
 - Calibrate Sensor 62
 - Zero Sensor 62
- PM Config softkeys
 - Connection Type 62
 - PM VXI-11 Device Name 62
 - Power Meter IP Address 62

- Power Meter IP Port 62
 - Point Trigger softkey 31
 - point-to-point time 246
 - polarity, external trigger 128
 - polarity, marker, setting 122
 - power
 - meter 58, 63
 - on, settings 19
 - peak-to-average, reducing 137
 - receptacle 11
 - search 74
 - sensor, models 60, 61
 - setting 29
 - softkeys 17, 19, 29–38, 73
 - supply, troubleshooting 235
 - switch 7
 - troubleshooting 235
 - power meter
 - configuration 63
 - U2000 Series 63
 - U2000A/01A/02A/04A 63
 - power meter configuration softkeys. *See* PM Config softkeys
 - power meter softkeys. *See* PM Config softkeys
 - Power Search Reference softkey 73
 - Power softkeys
 - On 19
 - On/Preset 17
 - Search 73
 - preferences, setting 17
 - preset
 - hardkey location 6
 - settings 19
 - troubleshooting 239
 - using 26
 - Preset softkeys
 - Language 19
 - List 38, 59
 - Preset 19
 - Prev REG softkey 80
 - Prev SEQ softkey 80
 - Proceed With Reconfiguration softkey 22
 - programming guide content xi
 - protection, DAC over range
 - baseband offset frequency 150
 - phase noise impairment 188
 - pulse
 - annunciator 9
 - characteristics 87
 - connector 12
 - marker, viewing 119
 - modulation 85
 - narrow 74
 - sync signal 32
 - video signal 32
 - Pulse hardkey 86
 - pulse modulation 3
 - Pulse softkeys 32, 86
 - Pulse/RF Blank softkey 115
 - PWT softkey 192
- ## Q
- Q connector 7
 - Q Offset softkey 155
 - quadrature adjustment 155
 - quadrature angle 92
 - Quadrature Angle Adjustment softkey 92, 155
 - queue, error 56
 - quick setup
 - Default softkey
 - settings 192
 - Quick Setup Softkeys 192
- ## R
- R annunciator 9
 - raised cosine filter. *See* nyquist filter
 - RAM 226, 227
 - real-time
 - AWGN
 - softkeys 179
 - I/Q Baseband AWGN softkeys 181
 - noise 178
 - phase noise 183
 - adjustments 187
 - DAC over range & scaling 188
 - description & plots 185
 - impairments 183
 - softkeys 184
 - rear panel
 - I/Q outputs 153
 - overview 11
 - Recall hardkey 51
 - Recall keys
 - hardkey 80
 - Instrument State 46, 49
 - Reg 80
 - State 49
 - recall register, troubleshooting 238
 - receiver test 190
 - rectangular clipping 138, 141
 - rectangular filter
 - definition 246
 - REF annunciator 9
 - REF IN connector 13
 - Ref Oscillator Ext Bandwidth key 30
 - Ref Oscillator Ext Freq key 30
 - Ref Oscillator Source softkey 29
 - reference oscillator, external 30
 - reference, using 76
 - references, content of xi

Index

regrowth, spectral 136
remote interface, emulate HP 3300A 80
Remote Language softkey 21, 23
remote operation annunciator 9
remote operation preferences 21
Rename File softkey 46
Rename Segment softkey 98
Reset & Run softkey 127
Restart on Trig softkey 127
Restore softkeys
 LAN Settings to Default Values 22
 System Settings to Default Values 19
resynchronize, multi-BBGs 163
Return hardkey 7
Reverse Power Protection softkey 19
Revert to Default Cal Settings softkey 157
RF
 blanking
 marker function 120
 settings, saving 111
 hardkey 6
 output
 configuring 29
 connector 6
 leveling, external 67–73
 troubleshooting 235
RF During Power Search softkey 73
RF Output softkey 152, 153
RFC NETBIOS Naming softkey 22
ringing 144
ripple 144
RMS 246
RMS softkey 73
Rohde & Scharz softkey 23
root 246
root cosine filter. *See* root nyquist filter
root mean square 246
Root Nyquist Filter
 definition 246
root nyquist filter
 definition 246
rotary knob 27
Route Connectors softkey 31, 86
Route To softkeys 32, 86
routing
 I/Q 92, 152
 marker
 ALC hold 112
 RF blanking 120
 saving settings 111
RPG test 241
runtime scaling 146

S

S annunciator 9

sales, Agilent offices 243
sample rate clock 15
sample rate softkey 125
Save hardkey 51
SAVE Seq Reg softkey 51
Save Setup To Header softkey 105
Scale Waveform Data softkey 143
scaling softkeys 143
SCPI
 enabling 22
 reference content xi
 softkey 23
screen saver settings 18
Screen Saver softkey 18
search, power 74
secure
 display 231
 mode 230
security 225
Security softkey 46
Segment Advance softkey 127
segment advance triggering 127
segments
 advance triggering 129
 file headers 105
 loading 98
 softkeys 98
 storing, loading, & playing 98
Select hardkey 27
Select Seq softkey 80
Select softkeys
 Color Palette 18
 Different Header 105, 109
 Header 105
 Internal File(s) to Copy to USB 50
 Reg 51
 Seq 51
 Waveform 38
self test 241
Sequence softkey 46, 105
sequences
 editing 103
 file headers 105
 marker control 123
 playing 104
 waveform 101
serial data, synchronizing 15
server, enabling 22
service
 Agilent offices 243
 guide content xi
 request annunciator 9
Set Marker softkeys 115
settings, persistent 246
settings, phase noise 187

- Show softkeys
 - Alpha Table 27
 - Waveform Sequence 101
 - Waveform Sequence Contents 101, 123
 - signal generator
 - modes 3
 - Signal Studio 2
 - signal studio licenses 24
 - sinewave 246
 - Single softkey 127
 - Single Sweep softkey 31
 - skew, I/Q 155
 - Sockets SCPI softkey 22
 - sockets, enabling 22
 - softkeys
 - definition of 246
 - help on 26
 - label area 10
 - location 4
 - See also* specific key
 - source settled signal 32
 - Source Settled softkey 32, 86
 - Span softkey 73
 - Specify Default Storage Path for User Media softkey 46
 - spectral regrowth 136
 - spectrum analyzer, troubleshooting signal loss 236
 - square root raised cosine filter. *See* root nyquist filter
 - Square softkey 86
 - standard, modulation 246
 - standby (yellow) LED 7
 - State softkey 46
 - states, persistent 246
 - step array (user flatness) 64
 - See also* user flatness correction
 - Step Dwell softkey 33, 78
 - Step Spacing softkey 33
 - step sweep
 - spacing 33
 - troubleshooting 238
 - using 33
 - Step/Knob Ratio softkey 19
 - Storage Type softkey 47, 55
 - Store To File softkey 48, 49
 - Stored Segments softkey 46, 105
 - Subnet Mask softkey 22
 - Sum softkey 152
 - sweep
 - annunciator 9
 - hardkey 31
 - linear 33
 - list parameters 39
 - list status information 39
 - logarithmic 33
 - manual control 42
 - mode 3
 - out connector 12, 32
 - out signal 32
 - softkeys 31–42, 86
 - step 33
 - troubleshooting 238
 - waveform, including 40
 - SWEEP hardkey 31
 - Sweep softkeys 31–42, 50, 86
 - swept output 31
 - switch, power 7
 - SWMAN annunciator 9
 - synchronize multi-BBGs 158
 - configure setup 161
 - equipment setup 161
 - resynchronize 163
 - system delay 160
 - system sync 160
 - trigger setup 160
 - system defaults, restoring 19
- ## T
- T annunciator 9
 - talker mode annunciator 9
 - TCP 247
 - TCP Keep Alive softkeys 22
 - TDMA digital modulation 195
 - terminator 247
 - test, self 241
 - tests, front panel 241
 - TETRA softkey 192
 - text area (on display) 10
 - text entry softkeys 98
 - time, dwell 245
 - time, setting 20
 - time/date reference point 20
 - Time/Date softkey 20
 - time-based license 20, 242
 - Timer Trigger softkey 31, 78
 - Toggle softkeys 123
 - Trig
 - in connector 12
 - out connector 12, 32
 - out signal 32
 - trigger
 - connectors 12
 - hardkey 5
 - initiating 5
 - multiple BBG sync 160
 - Trigger setup softkeys 79
 - Trigger softkeys
 - & Run 127
 - Doublet 86
 - Key 31
 - Out Polarity 31
 - Source 126

Index

- Triggered 86
- Type 126
- Triggered softkey 86
- triggering
 - gated 127, 130
 - multiple BBG sync 160
 - equipment setup 161
 - segment advance 127
 - softkeys 126
 - waveforms 126
- troubleshooting 233
- two tone 190, 214–219
- two tone softkeys 215
- two-tone softkeys 215
- two-tone waveform, setup 213
- type, modulation 246

U

- UNLEVEL annunciator 10
- unleveled operation 73
- UNLOCK annunciator 10
- Unspecified softkey 105
- UNT, option 3
- UNU, option 3
- UNW, option 3
- Up Directory softkey 46, 47, 50
- Update in Remote softkey 18
- urls 2, 20, 24, 243
- USB
 - connecting media 55
 - definition 247
 - device connector 13
 - host connector 4
 - keyboard, using 80
 - softkeys
 - File Manager 46, 47
 - Keyboard Control 80
 - to BBG Memory softkey 50
 - to Internal Storage softkey 50
 - troubleshooting 239
- Use softkeys
 - As 49
 - Current Directory As Default Path 46, 55
 - Only Internal Storage 46
 - Only USB Media 46
- user
 - documentation content xi
 - files, backup and restore 45
 - flatness correction 58
 - preset 26
 - preset, troubleshooting 239
- user FIR
 - definition 247
- User softkeys
 - Configure Power Meter 59

- Current Directory As Default Path 47
- Do Cal 59
- Flatness 29, 46
- Flatness Correction 59
- Flatness Corrections 50
- Span 73
- User 19

Utility hardkey 17

V

- vector operation 95, 164
- View Next Error Page softkey 56
- View Previous Error Page softkey 56
- volatile memory 96, 98
- volatile, definition 247
- VXI-11, enabling 22
- VXT-11 SCPI softkey 22

W

- Waveform 5-Pack
 - history, using 171
 - history, waveform files 171
 - licensing 164
 - licensing, installing 165
 - licensing, understanding 164
 - licensing, warning messages 175
 - licensing, waveform file 165
 - status messages 167
 - using 164
- Waveform softkeys
 - Licenses 24
 - Runtime Scaling 143
 - Segments 98
 - Sequences 101, 123
 - Utilities 143
 - Waveform 31, 38
- waveforms
 - clipping 133
 - file headers 105
 - from digital baseband waveform 144
 - in a sweep 40
 - license 24
 - markers 110, 111
 - memory 227
 - multiple BBG synchronization 158
 - multitone 220–223
 - overview 96
 - saving instrument state 52
 - scaling 142
 - segment softkeys 98
 - sequence 101
 - storing, loading, & playing 98
 - triggering 126
 - two-tone 214–219
 - Waveform 5-Pack 171

Web Server softkey 22
window settings, FIR filter 209
WINIT annunciator 10

Y

yellow LED 7

Z

Zoom softkeys 115

Index