

# **HP 8566B Spectrum Analyzer** 100 **Hz to 22** GHz

**Technical Data** 

Outstanding Precision and Capability



# The HP 8566B Spectrum Analyzer

Designed for bench and system use, the HP 8566B offers superior measurement speed, microwave frequency accuracy, and sensitivity. Measure low-level signals up to 22 GHz with narrow resolution bandwidths. Synthesizer stability virtually eliminates long-term drift and residual FM.

Frequency range is 100 Hz to 22 GHz with a dc-coupled input. Preselected external mixers extend this coverage from 26.5 to 75 GHz. Other external mixers allow measurement to 325 GHz.

An internal bus and microcomputer control make possible many powerful operating and data processing features, as well as flexibility under computer control. Sixteen Kbytes of user RAM are available for storing trace data, instrument states, and custom downloadable programs (DLPs). All displayed information can be sent directly to an HP-IB plotter when sweeptime is greater than or equal to 20 ms.

## Accurate Measurements

Amplitude measurement range extends from +30 to -135 dBm with a 90 dB calibrated display.

Less than 1 x 10<sup>-9</sup>/day frequency reference error and the spectrum analyzer selectivity allow high frequency accuracy even when you are measuring small signals in the presence of large ones.

# The Spectrum Analyzer That Keeps Getting Better

## **Turbo Speed Option**

Already a world leader in measurement speed, the HP 8566B can be made even faster with Option 002, which nearly doubles the internal processing speed of the analyzer. Some measurements can be made up to 50% faster, and overall throughput is typically improved by 5 to 25%. (Sweep speed is not affected by Option 002.)

The Turbo option is compatible with all HP 8566B accessories, and it can be added to any HP 8566B without affecting specifications. (An HP 8566A must first be upgraded to an HP 8566B.)

# **Accessories and Options**

By adding measurement accessories and options, the HP 8566B spectrum analyzer fits into many applications, including electromagnetic compatibility (EMC) testing, broadband signal surveillance, and component stimulusresponse testing. • *EMI* measurement accessories and software create systems for testing to commercial and military standards.

• Microwave tracking sources add scalar measurement capability.

• Preselected external mixers simplify millimeter-wave measurements from 26.5 to 75 GHz.

. Interactive test generator (ITG) soft-front-panel-based drivers speed software development.

• MIL-STD 45662A calibrations are available.

## **Custom Softkey Programming**

You can create complex measurement routines on an external controller, store the programs in user RAM, and execute them using a single custom softkey.


Simple measurement routines can be entered from the intrument front panel, stored in user RAM, and executed using a single custom softkey.

# **Turbo Speed Improvements**

Operation	Standard HP 8566B	Turbo HP 8566B	<b>Speed</b> Improvement
Trace Dump	1083 ms	<i>532</i> ms	51%
MKR AMPL	<i>8.4</i> ms	<i>3.7</i> ms	56%
<b>Harmonics</b> Test	1007 ms	782 ms	22%
FFT	473 ms	<i>243</i> ms	49%

The HP 8566B Microwave Spectrum Analyzer — Smart Enough to Make Its Own Decisions with Precision and Speed

One keystroke sends all CRT information directly to a plotter\*

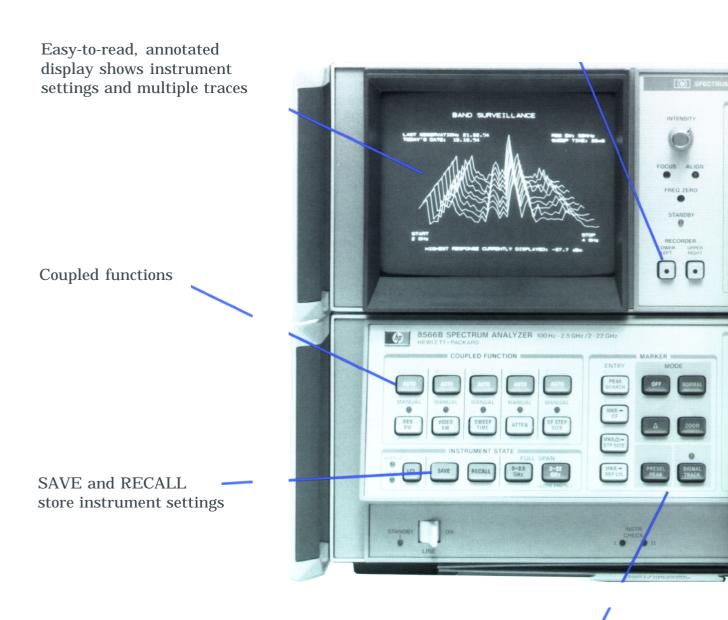

\* Instrument sweeptimes greater than or equal to 20 ms Measurement aids include four tunable markers for direct and relative signal measurements Powerful signal and traceprocessing functions perform complex data analysis






Dedicated keys make basic operation easy

Interactive function and data controls simplify operation

# **Today's HP 8566B Offers**

- Exceptional microwave performance
- Decision-making capability
- Enhanced processing speed
- Preselected millimeter coverage
- Advanced functions
- Downloadable programming capability
- Distributed processing with a computer
- Proven reliability, performance, and support

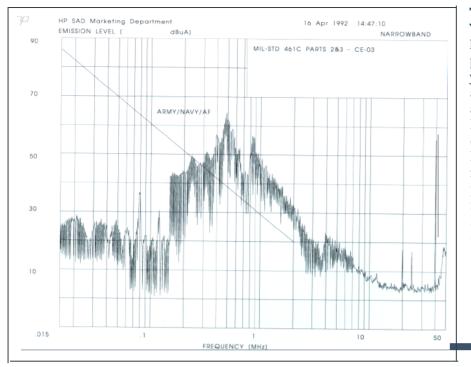

## Test Systems Tailored to Your Needs

For EM1 troubleshooting and pre-qualification testing, use your HP 8566B spectrum analyzer with components and accessories from HP's complete line of EM1 products. The many offerings include current probes, line impedance stabilization networks (LISNs), antennas, positioning equipment, EM1 measurement software, an RF preselector, and a quasi-peak adapter.

# **EMC Measurement** Solutions

## Commercial and MIL EM1 Receivers

The HP 8566B spectrum analyzer forms the heart of two powerful and flexible EM1 receivers. These receivers are ideal for commercial and military EM1 compliance testing from 20 Hz to 40 GHz.

The HP 8571A receiver is optimized for military EM1 testing, making both peak and average detection measurements using impulse bandwidths. The HP 85728 includes all the features and capabilities of the HP 85718, but adds quasi-peak detection and specialized IF bandwidths for commercial compliance measurements.

Both receivers offer  $\pm 2 \, dB$  absolute amplitude accuracy over their full 20 Hz to 22 GHz frequency range, as required by MIL-STD 461 and CISPR Publication 16. For higher frequency measurements, a 22 to 40 GHz block downconverter can be added. The receivers include a built-in, 1 to 26.5 GHz amplifier and a 20 Hz to 50 MHz input port with a built-in limiter and rugged attenuator. They are also compatible with HP's EM1 measurement software and complete line of test accessories.



# Accessories That Enhance Performance

# **Millimeter Mixers**

# **Preselected Mixers**

Harmonic Mixers


The HP 11970 series waveguide mixers are general-purpose external harmonic mixers. They offer flat frequency response and low conversion loss without

requiring external dc bias or


bands covering 18 to 110 GHz.

tuning adjustment. The HP 11970 series mixers are offered in six

The HP 11974 series preselected mixers eliminate the need for timeconsuming signal identification routines at millimeter frequencies. With preselection, no images or multiples are generated to confuse measurements. These external mixers allow you to quickly locate true signals, and they simplify software development for automated measurements. The HP 11974 series mixers are available in four bands covering 26.5 to 75 GHzJ

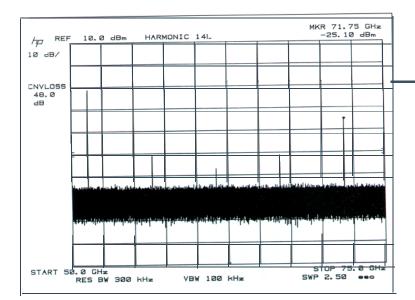

Preselected mixers eliminate images and multiples.

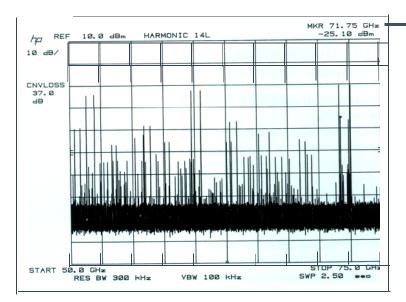

Harmonic mixing extends frequency range.



# **Tracking Sources**


Add high dynamic range scalar measurement capability to the HP 8566B. The HP 856448 and 856458 portable tracking sources allow you to use your spectrum analyzer for measuring transmission and reflection characteristics of devices. You can also characterize harmonic distortion, intermodulation distortion, spurious products, and more.



The tracking sources give the HP 8566B dynamic range greater than 125 dB up to 12.5 GHz and greater than 105 dB through 22 GHz.

Other features include:

- swept offset tracking for mixer testing and swept TOI measurements
- up to +10 dBm leveled output power
- standalone CW source capability

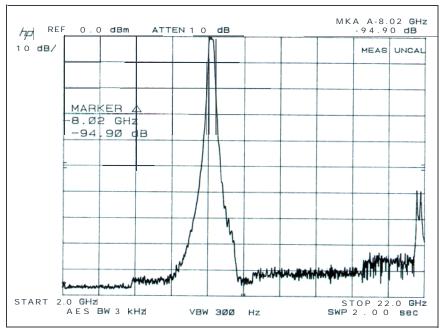



# **Microwave Preamplifier**

Boost the sensitivity of the HP 8566B spectrum analyzer with the HP 8449B microwave preamplifier. This low noise, high gain preamplifier has a frequency range of 1 to 26.5 GHzJ Sensitivity improvements of up to 25 dB allow you to detect and analyze very low level signals in dramatically reduced time, using wider bandwidths. Low return loss on the input and output ports of the preamplifier minimizes mismatch uncertainty.

# **Displayed Average Noise Level,**

0 dB Attenuation, 10 Hz RBW (characteristic)

1.0 to 2.5 GHz	-155 dBm
<b>2.0</b> to 5.8 GHz	-154 dBm
5.8 to 12.5 GHz	-150 dBm
12.5 to 18.6 GHz	-144 dBm
18.6 to 22 GHz	-140 dBm



# **Computers and Plotters**

The HP 8566B spectrum analyzer works with computers that support HP BASIC, including HP 9000 Series 200 and 300 computers and IBM PC/AT-compatible models.

The HP 7440 and 7550 plotters are recommended for use with the HP 8566B. Data can be sent directly from the analyzer to the plotter, without the need for a computer.

# **Specifications**

**Specifications** describe the instrument's warranted performance over the 0" to 55" C temperature range (unless otherwise noted), with autocoupled function operation and preselector tracking optimized. **Characteristics** provide information about non-warranted instrument performance.

# Frequency

Measurement Range 100 Hz to 22 GHz, dc-coupled input; up to 325 GHz with external mixers

# Frequency Reference Error

Aging Rate  $\triangleleft 1 \times 10^{-9}$ /day and  $\triangleleft 2.5 \times 10^{-7}$ /year Temperature Stability< 7 x 10 <sup>9</sup> over 0" to 55" C range Center Frequency 0 Hz to 22 GHz Center Frequency Readout Accuracy

**Spans**  $\leq$  **n** x 5 **MHz**  $\pm$ (2% of frequency span + frequency reference error x center frequency +1 0 Hz) **Spans**  $\Rightarrow$  **n** x 5 **MHz**  $\pm$ (2% of frequency span + n x 100 kHz + frequency reference error x center frequency) where n is the harmonic mixing number, depending on center frequency:

### n Center Frequency

- 1 100 Hz to 5.8 GHz
- 2 5.8 to 12.5 GHz
- 3 12.5 to 18.6 GHz
- 4 > 18.6 GHz

(After adjusting freq zero, add 30% of RES BW setting if error correction is not used.) **Zero Span**  $\pm$  (frequency reference error x center frequency)



# Frequency Span

0 Hz, 100 Hz to 22 GHz over IO division CRT horizontal axis; variable in approximately 1% increments. Two FULL SPAN keys select spans from 0 to 2.5 GHz and from 2 to 22 GHz.

### Frequency Span Readout Accuracy

 $\mbox{Spans} \leq n \ x \ 5 \ \mbox{MHz} \ \pm 1 \ \%$  of indicated frequency separation

 $\textbf{Spans} \mathrel{>} n \times 5 \ \textbf{MHz} \ \underline{\pm}3\%$  of indicated frequency separation

Start or Stop Frequency Same as center frequency

### Resolution

**Resolution Bandwidth** 3 dB bandwidths of IO Hz to 3 MHz in a 1, 3 10 sequence. Bandwidth may be selected manually or coupled to frequency span (AUTO mode).

## 3 dB Bandwidth Accuracy

	nuoy
3 MHz	<u>+</u> 20%
3 kHz to 1 MHz	<u>+</u> 10%
10 Hz to 1 kHz	<u>+</u> 20%
(30 kHz and 100 kH	z bandwidth accuracy figures
apply only with $\leq 90^{\circ}$	% relative humidity, $\leq 40^{\circ}$ C.)

# 60 dB/3 dB Bandwidth Selectivity Ratio

100 kHz to 3 MHz	⊲ 15:1		
3 kHz to 30 kHz	⊲ 13:1		
30 Hz to 1 <b>kHz</b>	⊲ 12:1		
(60 dB points on IO Hz bandwidth are			
separated by ⊲ 100 Hz.)			

## **Bandwidth Shape**

Synchronously tuned, approximately Gaussian

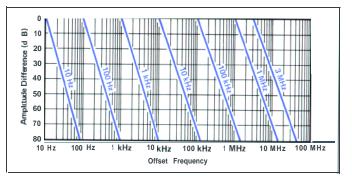


Fig. 1. Typical spectrum analyzer resolution

## Stability

**Residual FM** (typical) For fundamental mixing  $(n=1) \triangleleft 50 \text{ kHz}$  peak-to-peak, freq. span  $\Rightarrow 5 \text{ MHz}$ . **Drift** Because analyzer is phase-locked at beginning of each sweep, drift occurs only during time of one sweep.

Frequency	Span
⊴ 100 <b>kHz</b>	
100 <b>kHz-5</b> M	1Hz
≥ 5 MHz	

Center Frequency Drift' < IO Hz/min of sweeptime ⊲ 500 Hz/min of sweeptime

≥ 5 MHz ⊲ 5 KHz/min of sweeptime
 Typical, after 1 hr warmup at stabilized temp

COUPLED FUNCTION not required.

## **Spectral Purity**

Noise Sidebands (for frequency span ≤ 25 kHz--except 100 kHz offset--and center frequencyfrom 100 Hz to 5.8 GHz)Offset from Carrier320 Hz-80 dBc/Hz1 kHz-85 dBc/HzIO kHz-90 dBc/Hz100 kHz-105 dBc/Hz

## **Typical Noise Sideband Performance**

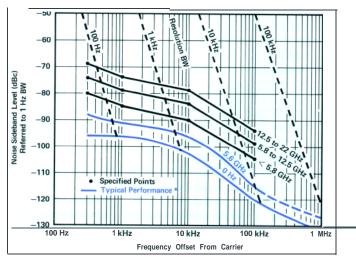


Fig. 2. Single sideband noise normalized to 1 Hz BW vs offset from carrier

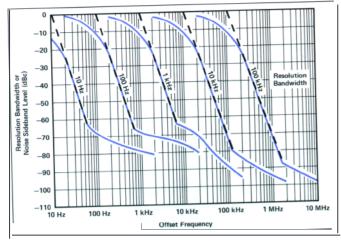


Fig. 3. Typical analyzer and SSB noise at 5.0 GHz center frequency. May be limited by average noise level.

#### **Power-Line-Related Sidebands**

(for line conditions specfied in Power Requirements section)

SIDEBANDS

SIDEDANDO					
Offset		Center	requency	y	
from Carrier	≤100 MHz	> 100 MHz to 5.8 GHz	6.8 to 12.6 GHz	12.6 to 18.6 GHz	18.6 <b>to</b> 22 GHz
<b>&lt;360</b> Hz	-70 dBc	-60 dBc	-64dBc*	-60 <b>dBc</b> *	-58dBc*
360 kHz to 2 kHz	-75 dBc	75dBc*	-69dBc*	-65dBc*	-63dBc*
⊳2 kHz	-80dBc	-80dBc*	-74dBc*	-70dBc*	-63dBc*
					Typical'

## **Amplitude**

#### **Measurement Range**

Measurement range is the total amplitude range over which the analyzer can measure signal responses. The low value is determined by sensitivity (10 Hz RBW and 0  $dB\,\text{RF}$  input attenuation) and the high value by damage level. Range

#### **Tuned Frequency**

Non-preselected	
100 Hz to 50 <b>kHz</b>	– 95 to + 30 dBm
50 kHz to 1 MHz	– 112 to + 30 <b>dBm</b>
1 MHz to 2.5 GHz	- 134 to + 30 dBm
Preselected	100 to 100 dBm
2.0 to <b>5.8 GHz</b>	– 132 to + 30 dBm
5.8 to 12.5 GHz	– 125 to + 30 dBm
12.5 to 18.6 GHz	— 119 to + 30 dBm
<b>18.6</b> to 22 GHz	– 114 to + 30 dBm

## **Displayed Values**

Scale (over a 10 division CRT vertical axis with 0 dB reference level at top graticule line)

#### Calibration

Log 10 dB/div for 90 dB display from reference level.			
Expanded from reference level:			
5 dB/div for 50 <b>dB</b> display			
2 dB/div for 20 dB display			
1 dB/div for 10 <b>dB</b> display			
Linear 10% of ref level/div when calibrated voltage			

## **Reference Level**

#### Range

- Log +30.0 to -99.9 dBm or equivalent in dBmV, dBµV, volts. Readout expandable to +60.0 dBm to -119.9 dBm  $(-139.9 \text{ dBm} \text{ for } \le 1 \text{ kHzRBW})^*$
- Linear 7.07 V to 2.2 µV full scale. Readout expandableto 223.6 V to 2.2  $\mu$ V (0.22  $\mu$ V for ⊲ 1 kHz RBW)\*

Maximum total input power not to exceed +30 dBm damage level

#### Accuracy

The sum of the following factors determines the accuracy of the reference level readout. Measurement technique used after calibration with CAL signal determines applicability of uncertainty sources. Specifications given with preselector tracking optimized using MARKER PRESELECTOR PEAK.

With corrected readout (SHIFT W and SHIFT X executed just prior to measurement), 20" to 30° C temperature range, and minimum one hour warmup time.

#### Calibrator Uncertainty ±0.3 dB Fr

Frequency Response (Flatness) Uncertainty			
(10 <b>dB</b> attenuation)			
100 Hz to 2.5 GHz			
2.0 to 12.5 GHz	±1.7 dB		
12.5 to 20 GHz	±2.2 dB		
20 to 22.0 GHz	±3.0 dB		
Cumulative, 100 Hz t	o 20 GHz f2.2 dB		
Absolute Amplitude	e Calibration Uncertainty		
The uncertainty of se	etting the frequency response		
curve absolutely whe	en using the internal		
CAL signal or other of	calibration signal in the		
100 Hz to 2.5 GHz b	and (10 <b>dB</b> input attenuation).		
±0.6 dB			
Resolution Bandwidth Switching Uncertainty			
Referenced to 1 M			
10 Hz	±1.1 dB		
<b>30</b> Hz	±0.4 dB		
100 Hz to 1 MHz f0.2 dB			
3 MHz f0.2 dB			
Log Scale Switching Uncertainty ±0.1 dB			
Log Fidelity			
	0.1 dB/dB over 0 to 80 dB display		
Cumulative			
10 Hz RBW			
≥ <b>30</b> Hz RBW			
	⊴ ± <b>1</b> .O <b>dB</b> over 0 to 80 <b>dB</b>		
Linear Fidelity			
	9-1/2 divisions of the display		
IF Gain Uncertai	inty Reference to -10 dBm		

IF Gain Uncertainty Reference to -10 dBm; reference level with 10 dB input attenuation.

	Reference Level
RBW ≥ 3 <b>kHz</b>	0 to -59.9 <b>dBm</b> ≤ ± 0.3 <b>dB</b>
	$-60 \text{ to } -100 \text{ dBm} \le \pm 1.0 \text{ dB}$
RBW 100 Hz-I kHz	0 to -79.9 dBm ≤ ± 0.3 dB
	$-80 \text{ to } -100 \text{ dBm} \le \pm 1.0 \text{ dB}$
RBW 30 Hz	0 to -79.9 dBm $\leq \pm 0.3$ dB
	-80 to -100 <b>dBm</b> ≤ ± 2.0 <b>dB</b>
RBW 10 Hz	0 to -79.9 <b>dBm</b> ≤±1.0 <b>dB</b>
	-80 to -100 dBm $\leq \pm 2.0$ dB



### Log Digitization Uncertainty

10 dB/div	± 0.2 dB
5 dB/div	fO.IdB
2 dB/div	± 0.04 dB
1 dB/div	± 0.02 dB

Linear Digitization Uncertainty  $\pm$  0.2% of ref level

Error Correction Accuracy (applicable when SHIFT W and SHIFT X are executed)  $\pm 0.4 \text{ dB}$ 


**Reference Line Accuracy** Equals the sum of reference level accuracy plus the scale fidelity between the reference level and the reference line level.

## **Dynamic Range**

**Spurious Responses** (signals generated by the analyzer due to input signals) for signals  $\leq$ -40 dBm at the input mixer, all harmonic and intermodulation distortion > 70 dB below input signal.

Second Harmonic Distortion (for mixer levels ≤ -40 dBm)

100 Hz to 50 MHz	⊲ -70 dBd
50 to 700 MHz	⊲ -80 dBc
700 MHz to 2.5 GHz	⊲ -70 dBc
For mixer levels ⊴ -10 dBm	
2 to 22 GHz	< -100 dBc

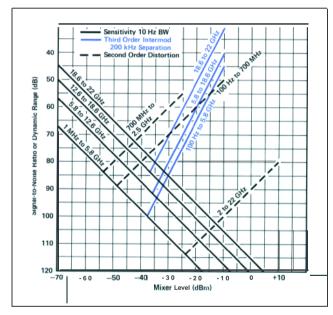



## Third Order Intermodulation Distortion

Third Order Intercept (TOI) 100 Hz to 5 MHz

 5 MHz to 5.8 GHz
 > + 7 dBmi

 5.8 GHz to 18.6 GHz
 > + 5 dBmi

 18.6 to 22 GHz
 > + 5 dBmi (typical)

 2 to 22 GHz, for > 100 MHz
 > + 50 dBmi (typical)

 signal separation
 > + 50 dBmi (typical)

> + 5 dBm

#### Image, Multiple, and Out-of-Band Responses

Image responses are due to input signals that are two times the IF frequency above or below the tuned frequency. Multiple responses are due to input signals mixing with more than one LO harmonic. Out-of-band responses are due to input signals outside of the selected frequency band.

Applied	Tuned
Frequency	Frequency
	0 0 5 0

 (GHz)
 0-2.5
 2.0-5.8
 5.8-12.5
 12.5-18.6
 18.6-22.0

 0-2.5
 NA
 -60
 dBd
 -60
 dBc
 -70
 dBc
 40</

**Residual Responses** (signals displayed by the analyzer independent of input signals), 0 **dB** input attenuation, no input signal.

۱*

\*Limited by the appropriate DANL or -100 dBm, whichever is greater. Gain Compression

⊲ 1 .O dB, 100 Hz to 22 GHz, with ⊴ -5 dBm at input mixer

#### **Displayed Average Noise Level (Sensitivity)**

0 dB input attenuation, 10 Hz RBW	
100 Hz to 50 <b>kHz</b>	⊲ -95 <b>dBm</b>
50 <b>kHz</b> to 1 .O MHz	< -112 dBm
1 .O MHz to 2.5 GHz	< -134 dBm
2.0 to 5.8 GHz	⊲ -132 <b>dBm</b>
5.8 to 12.5 GHz	⊲ -125 <b>dBm</b>
12.5 to 18.6 GHz	< –119 dBm
18.6 to 22 GHz	< -114 dBm

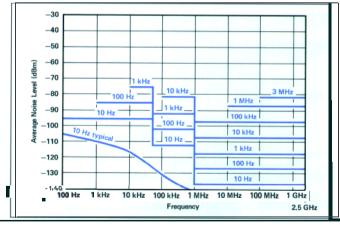


Fig. 5. Specified average displayed noise level, 100 Hz to 2.5 GHz, non-preselected tuning range

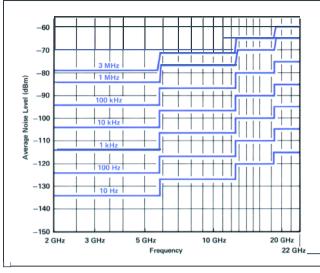


Fig. 6. Specified average displayed noise level, 2.0 to 22 GHz, preselected tuning range

#### Marker

(frequency and amplitude are read out continuously)

Marker Type	Frequency Accuracy
Normal	same as center frequency accuracy
Delta	same as frequency span accuracy
	Amplitude Accuracy
Normal	same as reference level accuracy +
	scale fidelity between the reference
	level and marker position
Delta	same as frequency response
	uncertainty and scale fidelity
	between two markers

#### Sweep Time Accuracy (1 µs to 1500s full sweep)

 $\leq$  200 second sweep time,  $\pm$  10%

> 200 second sweep time,  $\pm 30\%$ 

#### Inputs

RF Input 100 Hz to 22 GHz, precision type-N female connector, dc-coupled

## Maximum Input Level

- ac Continuous power: +30 dBm from 50 ohm source Mixer protected by diode limiter, 100 Hz-2.5 GHz Pulse power: ≤ 100 W, 1 0µs pulse width with ≥ 50 dB input attenuation (I 0 dBm peak power to input mixer)
  - ⊲ 100 mA damage level

Input Attenuator0 to 70 dB in 10 dB steps

SWR (typical)	Tune Frequency		
Input	100Hzto	2 GHz to	5.8 GHz to
Attenuation	2.5 <b>GHz</b>	5.8 <b>GHz</b>	22 <b>GHz</b>
10 dB	1.2	1.5	1.9
0 dB*	2.3	3.0	3.0

'when tuned to within  $\pm 3~\text{MHz}$  of signal

## IF Input

dc

Maximum Input Level

- ac +10 dBm continuous power from 50 ohm source
- dc 20 V with rise time of  $\triangleleft$  1 V/µs

**External Sweep Trigger Input** (rear panel) Must be > 2.4 V (5 V max), 1 kohm nominal input impedance. **External Frequency Reference Input** Must equal 5 MHz  $\pm$  25 Hz or 10 MHz  $\pm$ 50 Hz, 0 to +10 dBm, 50 ohm nominal input impedance. Analyzer performance will be degraded unless frequency reference phase noise and spurious signals are <-140 dBd single sideband (1 Hz) referred to 10 MHz at a 100 Hz to 10 kHz offset. **Quasi-Peak** (rear panel; nominal values)

Video Input 0 to 2 V, 139 ohm input impedance 21.4 MHz IF Input Nominally -11 dBm with 10 dB input attenuation, 50 ohm input impedance

# Outputs

Calibrator (front panel)

100 MHz ± (frequency reference error x 100 MHz) -10 dBm ± 0.3 dB; 50 ohm impedance, nominal

#### **1st LO** (front panel)

2.3 to 6.1 GHz; > +5 dBm;

- 50 ohm impedance, nominal
- Sweep and Tune Output (rear panel)

-1 V/GHz of tuned frequency  $\pm$  (2% + 10 mV) 10 kohm impedance, nominal

# **Display Outputs** (typical parameters)

X, Y, and Z outputs for auxiliary CRT displays.

- X, Y 1 V for full deflection
- Z 0 to 1 V intensity modulation, -1 V blank
- BLANK TTL level > 2.4 V for blanking

# Compatible with most oscilloscopes.

Recorder Outputs (typical parameters)

Outputs to drive all current HP X-Y recorders using positive **pencoils** or TTL pen uplift.

Horizontal Sweep Output (X-axis)

A voltage proportional to the horizontal sweep of the frequency sweep generator. 0 V for left edge, +10 V for right edge; 1.7 kohm impedance, nominal. **Video Output** (Y-axis)

Detected video output (before A-D conversion) proportional to vertical deflection of the CRT trace 100 mV/div from 0 to 1 V;  $\leq$  475 ohm impedance, nominal.

#### Penlift Output (Z-axis)

During sweep, pen down 0 V from 10 ohm source During retrace, pen up +15 V from 10 kohm source

21.4 MHz Output (rear panel, typical)

21.4 MHz; 50 ohm impedance, nominal: -20 **dBm** for a signal at reference level. In log scales, the IF output logarithmically related to RF input signal; in linear, the output is linearly related.

Frequency Reference (rear panel, typical) 10.000 MHz, 0 dBm; 50 ohm output impedance 10 MHz Output (rear panel, typical) ≥ 5 dBm to ohm output impedance Video Output 0 to 2 V, > 10 ohm output impedance

## Displav

**Cathode Ray Tube** Post deflection accelerator, aluminized **P31** phosphor, electrostatic focus and deflection.

**Viewing Area** Approximately 9.6 cm vertically by 11.9 cm horizontally (3.8 in x 4.7 in)



# **General Specifications**

# **Environmental**

#### Temperature

Operation 0" to 55" C Storage -40" to 75" c Increased internal temperatures may result if the rear panel air filters are not cleaned regularly.

#### Altitude

**Operation** ≤ **4,572** m (15,000 ft) Storage ≤ 15,240 m (50,000 ft)

**Power Requirements** 50 to 60 Hz; 100,200, 120,220, or 240 V (+5%, -10%); approximately 650 VA (40 VA in standby). 400 Hz operation with Option 400. Humidity

**Operation** Type tested to 95% relative humidity, 25" to 40" C, except as noted in electrical specifications.

Storage 5% to 90% relative humidity, 0° to 40° C

EMI Conducted and radiated interference is within the requirements of MIL-STD-461C, Part 7 RE02 and CEO3 (Air Force), and CISPR Publication 11; VDE 0871 and FTZ 526/527/79.

#### Warm-Up Time

Operation Requires 30 minute warm-up from cold start, 0" to 55" C. Internal temperature equilibrium is reached after 2-hour warm-up at stable outside temperature.


Frequency Reference (typical)


Frequency reference aging rate attained after 24 hour warm-up from cold start at 25" C. Frequency is within 1 x 10-8 of final stabilized frequency within 30 minutes.

#### Weight

Total, net	50 kg (112 lb)
RF section, net	29 kg (65 lb)
IF display section, net	21 kg (47 lb)
RF section, shipping	35 kg (78 lb)
IF display section, shipping	27 kg (60 lb)

#### **Dimensions**

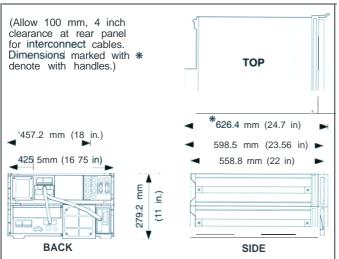





# **Remote Operation**

The standard HP 8566B operates on the Hewlett-Packard Interface Bus (HP-IB). All analyzer control settings (with the exception of VIDEO TRIGGER LEVEL, FOCUS, ALIGN, INTENSITY, FREQ ZERO, AMPTD CAL, and LINE power) are remotely programmable. Function values, marker frequency/ amplitude.and A/B traces may be output; CRT labels and graphics may be input.

LCL Returns analyzer to local control, if not locked out by controller.

## Service Request

SHIFT r calls an HP-IB request for service.

#### **HP-IB** Interface Functions

SH1, AH1, T6, L4, SRI, RL1, PPO, DC1, CI, C2, C3, C28, E2

#### Options

All specifications for options are identical to standard HP 85668 except as noted.

400 Hz Power Line Frequency Operation (Option 400) **Power Line Related Sidebands** 

(center frequency from 100 Hz to 5.8 GHz)		
Offset from Carr	ier Sideband Level	
⊴ 2 kHz	-55 <b>dBc</b>	
2 kHz to 5.5 kHz	-65 <b>dB</b> d	
<b>Power Requirements</b>	S	
Line frequency	400 Hz ±10% line frequency	
	(50 to 60 Hz operation for	
	servicing only)	
Line voltage	100 to 120 v (+5%, -10%)	
Operating Temperature Range		
400 Hz	0" to 55" c	
50 Hz to 60 Hz (s	ervice only	

50 Hz to 60 Hz (service only, not for extended periods) 0" to 40° C

Fig.7. Instrument dimensions with and without handles



# **Ordering Information**

HP 8566B Sp	ectrum Analyzer 100 Hz to 22 GHz
<b>Option R02</b>	Turbo retrofit kit for any HP 8566B
Option 002	Turbo option for faster measurements
Option 010	Rack mount slide kit
Option 016	Installed EM1 receiver functions
Option 031	German operating manual
Option 080	Information card in Japanese
Option 081	Information card in French
Option 1BN	MIL-STD 45662A calibration certification
Option 1BP	MIL-STD 45662A calibration certification
option ibi	with test data
<b>Option 400</b>	400 Hz operation
Option 462	100 Hz, 1 kHz, and 1 MHz
option 102	Impulse bandwidth filters for EM1 measurements
Option 908	Rack flange kit without handles
Option 910	Extra operating and test and adjustment manuals
Option 913	Rack flange kit with handles
Option 915	Troubleshooting and repair manual set
Option W30	3-year customer return repair
Option W32	3-year customer return calibration
Option W52	5-year customer return repair
Option W50	5-year customer return calibration
	5-year customer return tanbration
HP 8566AB	Retrofit kit to convert HP 8566A to HP 8566B
Recommende	d Accessories
HP 85644A	Tracking source 300 kHz to 6.5 GHz
HP 85645A	Tracking source 300 kHz to 26.5 GHz
HP 8449B	Preamplifier 1 to 26.5 GHz
HP 11975A	Amplifier 2 to 8 GHz
111 110704	
Preselected M	Aixers
HP 11974A	26.5 to 40 GHz preselected mixer
HP 11974Q	33 to 50 GHz preselected mixer
HP 11974U	40 to 60 GHz preselected mixer
HP 11974V	50 to 75 GHz preselected mixer
HP 11974	•
Option 003	Delete power supply
Harmonic Mi	xers*
HP 11970K	18 to 26.5 GHz mixer
HP 11970A	26.5 to 40 GHz mixer
HP 11970Q	33 to 50 GHz mixer
HP 11970T	18 to 40 GHz mixers, hardwood case, cables,tools
Option 001	Add 40 to 60 GHz mixer
Option 002	Add 33 to 50 GHz mixers
HP 11970U	40 to 60 GHz mixer
HP 11970V	50 to 75 GHz mixer
HP 11970W	75 to 110 GHz mixer
Option 009	Mixer connection set adds three l-meter low-loss

**Option 009** Mixer connection set adds three l-meter low-loss SMA cables, wrench, Allen screw driver for any HP 11970 series mixer.

\* For more information about other mixers, contact your local HP sales office.

United States: Hewlett-Packard Company 4 Choke Cherry Road Rockville, MD 20850 (301) 670 4300

Hewlett-Packard Company 5201 Tollview Drive Rolling Meadows, IL 60008 (708) 255 9800

Hewlett-Packard Company 5651 W. Manchester Los Angeles, CA 90045 (213) 337 8035

Hewlett-Packard Company 2000 South Park Place Atlanta, GA 30339 (404) 980 7351

Canada: Hewlett-Packard Ltd. 6877 Goreway Drive Mississauga, Ontario L4V 1M8 (416) 678 9430

Europe: Hewlett-Packard European Marketing Centre P.O. Box 999 1180 AZ Amstelveen The Netherlands (31) 20 547 9999

Japan: Yokogawa-Hewlett-Packard Ltd. 15-7, Nishi Shinjuku 4 Chome Shinjuku-ku Tokyo 160, Japan (03) 53711315

Latin America Latin American Region Headquarters Monte Pelvoux No. 111 Lomas de Chapultepec 11000 Mexico, D.F. (525) 202 0155

Australia/New Zealand: Hewlett-Packard Australia Ltd 31-41 Joseph Street Blackburn, Victoria 3130 Australia (A.C.N. 004 394 763) (03) 895 2895

Far East: Asia Pacific Hewlett-Packard Asia Pacific Ltd 22/F Bond Centre, West Tower 89 Queensway, Central, Hong Kong (852) 848 7777

For more information, call your local HP sales office listed in your telephone directory or an HP regional office listed below for the location of your nearest sales office.

Data subject to change Printed in U.S.A. 4/92 5091-33853