

Installation Note

**Agilent Technologies ESA E4401B/E4411A/E4411B
Spectrum Analyzers**

1.5 GHz Tracking Generator Retrofit Kit

50 Ω Retrofit Kit (Option 1DN)

75 Ω Retrofit Kit (Option 1DQ)



Agilent Technologies
Innovating the HP Way

Agilent Part Number E4411-90051

Printed in USA December 1999 Supersedes P/N E4411-90020

Notice.

The information contained in this document is subject to change without notice.

Agilent Technologies makes no warranty of any kind with regard to this material, including but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Tracking Generator Retrofit Kit

Products Affected:	E4401B E4411A E4411B
Serial Numbers:	US00000000/US99999999
To Be Performed By:	(x) Agilent Service Center (x) Personnel Qualified by Agilent (x) Customer
Estimated Installation Time:	1 Hour
Estimated Verification Time:	2 Hours

Introduction

These kits contain the parts and instructions to install a 50 Ω Tracking Generator (Option 1DN) or a 75 Ω Tracking Generator (Option 1DQ). A 75 Ω Tracking Generator should not be installed in an analyzer with a 50 Ω input. Similarly, a 50 Ω Tracking Generator should not be installed in an analyzer with a 75 Ω input.

Installation Kit Parts List

Table 1. 50 Ω Tracking Generator Kit (Option 1DN) E4401-60175

Item	Quantity	Description	Part Number
1	1	Board Assembly Tracking Generator, 50 Ω	E4401-60128
2	1	Adapter, Type-N(m) to STET (f), 50 Ω	1250-0780
3	4	Screw, M3 x 8 mm (crest washer - pan head - TORX)	0515-0372
4	1	Installation Note (this document)	E4411-90051

Table 2. 75 Ω Tracking Generator Kit (Option 1DQ) E4401-60176

Item	Quantity	Description	Part Number
1	1	Board Assembly Tracking Generator, 75 Ω	E4401-60129
2	1	Adapter, BNC(m) to F(f), 75 Ω	1250-2477
3	4	Screw, M3 x 8 mm (crest washer - pan head - TORX)	0515-0372
4	1	Installation Note (this document)	E4411-90051

Tools Required

- T-8 TORX screwdriver
- T-10 TORX screwdriver
- T-15 TORX screwdriver
- Spectrum analyzer, microwave
- 50 Ω termination, 2 required (Option 1DN only)
- 75 Ω termination, 2 required (Option 1DQ only)
- Power meter
- RF Power sensor
- Power sensor, 75 Ω (Option 1DQ only)
- Digital voltmeter (Option 1DN only)
- BNC (f) to dual banana plug (Option 1DN only)
- Cable, BNC 91 cm (36 in)
- Adapter, Type-N tee, (m)(f)(f) (Option 1DN only)
- Adapter, Type-N(m) to BNC (f) (Option 1DN only)
- Adapter, BNC(m) to Type-N (f) 75 Ω , 2 required (Option 1DQ only)
- Cable, Type-N, 62 cm (24 in)
- Cable, BNC, 23 cm (9 in)
- Cable, BNC, 122 cm (48 in)
- Torque driver (Torque driver requirements are shown in Table 3.)

Installation Procedure

WARNING Before you disassemble the instrument, turn the power switch OFF and unplug the instrument. Failure to unplug the instrument can result in personal injury.

CAUTION Electrostatic discharge (ESD) can damage or destroy electronic components. All work on electronic assemblies should be performed at a static-safe workstation. Refer to the documentation that pertains to your instrument for information about static-safe workstations and ordering static-safe accessories.

To avoid potential RFI leakage and prevent connector damage, tighten screws and RF coax cable connectors to the following values:


Table 3. Torque Settings

Item	Torque in-lb	Torque N-cm
SMA connectors	8.5	95
SMC connectors	5.5	62
3-mm, T-10 TORX screws	9.0	101
3.5-mm, T-10 TORX screws	14	157
4-mm, T-15 TORX screws	21	236
Pozidrive Screws	14	157

Remove Rear Frame and Outer Cover

1. Disconnect the ac power cord from the spectrum analyzer.
2. Refer to Figure 1. Carefully put the analyzer on the work surface with the front frame, (2) and (3), facing down.
3. Position the handle (4) as shown in the figure.
4. Remove the four screws (5) that hold the rear frame (6) and outer cover (7) in place.
5. Lift the instrument rear frame (6) and outer cover (7) up and off of the instrument and set them aside.

Figure 1. Remove Rear Frame and Outer Cover

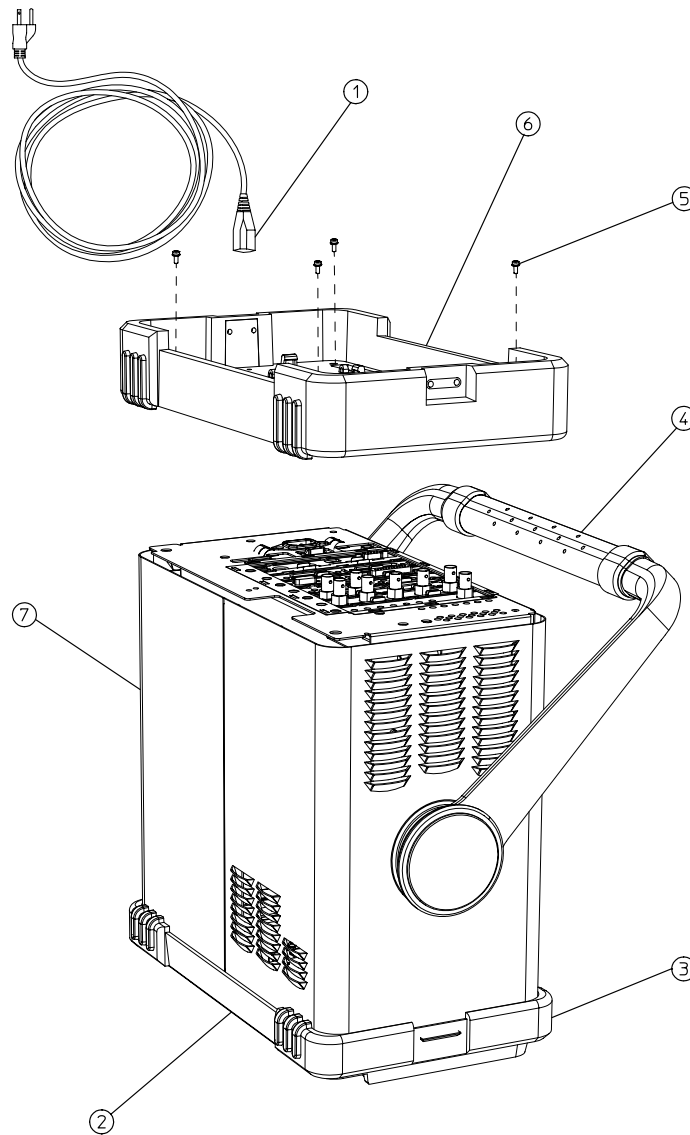


dl71b

Remove Chassis Cover

6. Refer to Figure 2. Remove the screws (2 and 3) attaching the chassis cover (1) to the chassis.
7. Remove the chassis cover from the chassis.

Figure 2. Remove Chassis Cover

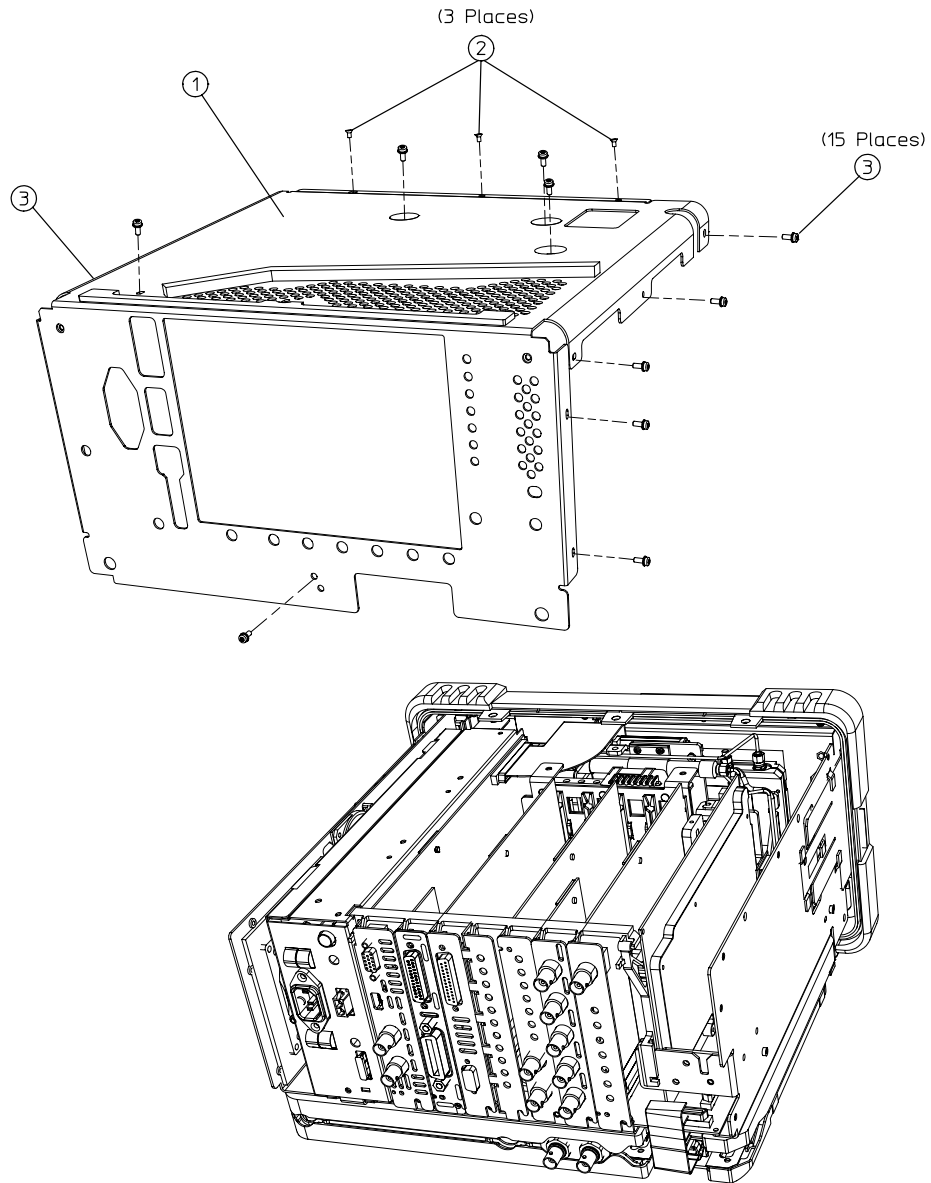


dn73b

Remove Front Frame and Install Tracking Generator

8. Refer to Figure 3. Remove the two screws on the bottom side (1) of the instrument that secure the front frame to the RF assembly.
9. Place the instrument with the top side facing up. Remove the two screws (2) that secure the front frame subpanel to the chassis sides.

Figure 3. Remove Front Frame

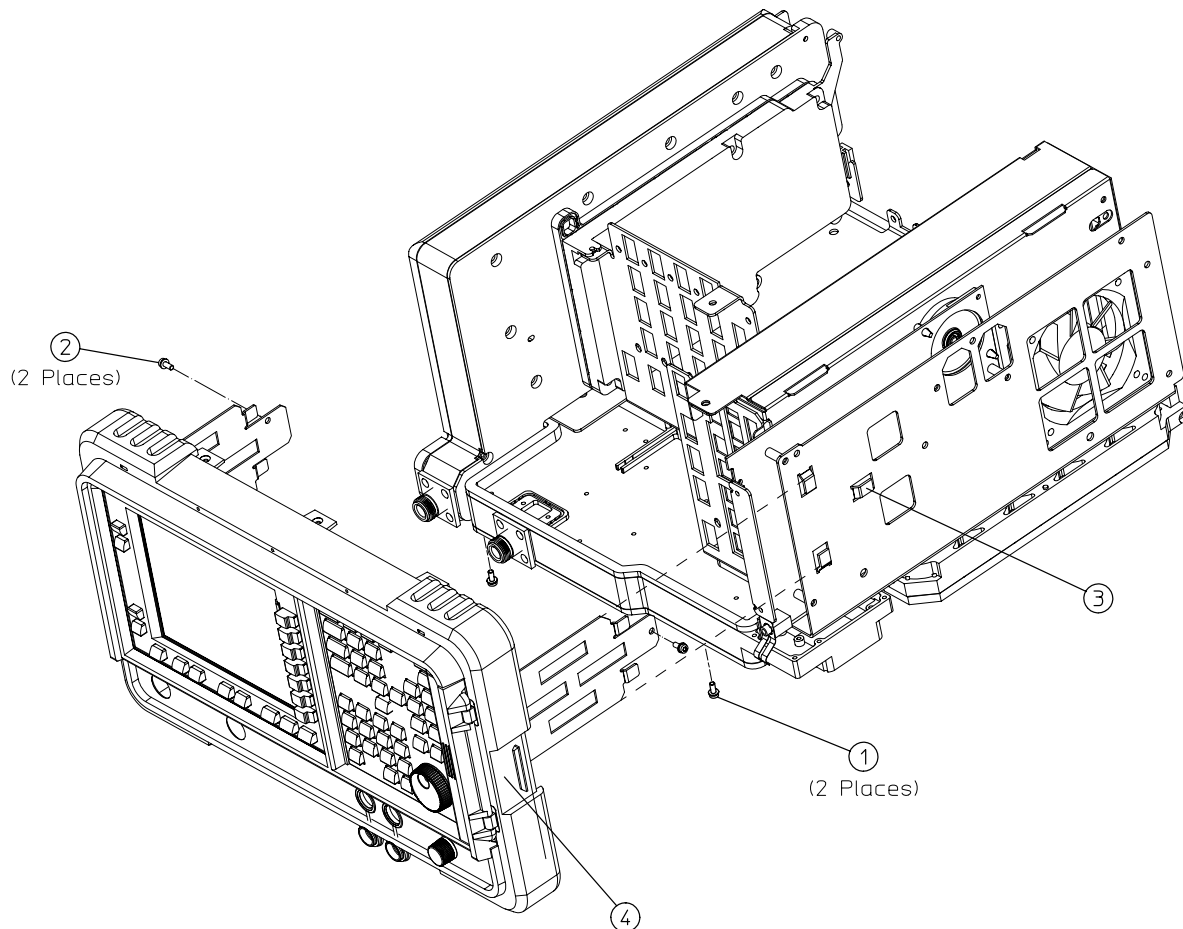


dn77a

10. Slide the front frame forward until it latches. Disengage the latches on each side of the instrument by sliding the front frame back toward the instrument a small amount and then gently pulling out on the latch tabs (3).
11. Slide the front frame forward just far enough to reach the ribbon connector attached to J2 on the front panel keyboard printed circuit board. Disconnect the ribbon cable from J2.
12. Remove the front frame and position it with the display down. With a flat-blade screwdriver, carefully press the side tab of the hole plug in the tracking generator RF Out connector hole (from the inside of the front panel) and push the plug out of the hole. Discard the hole plug and set the front panel assembly aside.

13. Refer to Figure 4. Remove the IF bracket by removing four screws (3). This bracket is located in back of the aluminum protrusion at (4). Discard the bracket.
14. Carefully insert the tracking generator assembly (2) into the motherboard.
15. Insert and attach the four screws (1) that secure the tracking generator to the chassis. These screws are supplied in this kit. Torque these screws to 101 N-cm (9 in-lb.).

Figure 4. Remove the IF Bracket and Install the Tracking Generator

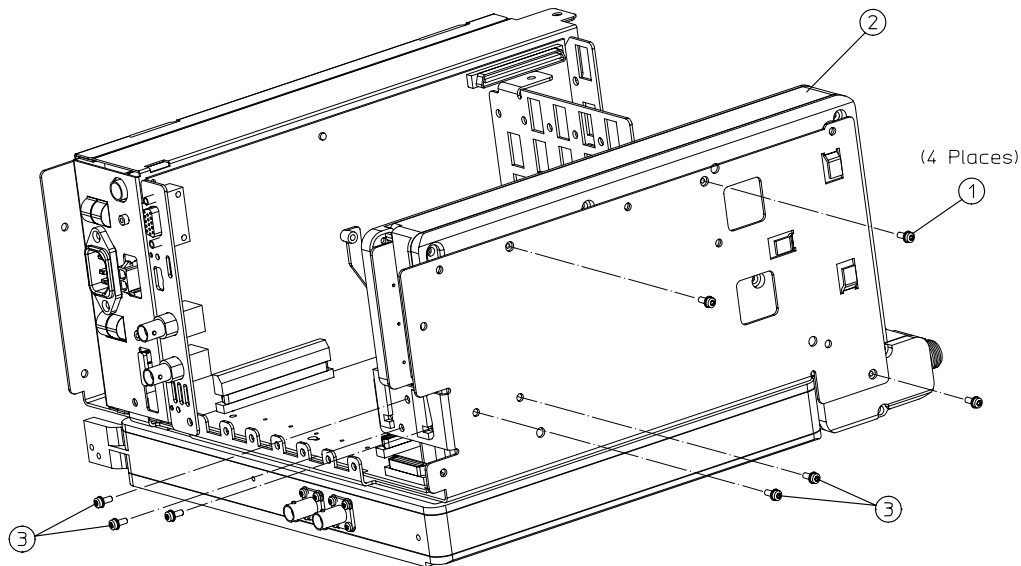

dn73a

Replace Front Frame

16. Make sure the water seal is still in place around the output connector hole on the front panel assembly.
17. Carefully slide the front frame onto the chassis and attach the ribbon cable to connector A2 on the front panel keyboard printed circuit board. Make sure that the ribbon cable is not pinched between assemblies.
18. Refer to Figure 3 and replace the four screws that secure the front frame to the chassis at locations (1), (2) and (3). Torque these screws to 9 in-lb (101 N-cm).

Replace Chassis Cover

19. Refer to Figure 2. Carefully position the chassis cover on the instrument as shown.
20. Replace the 15 pan head screws (3) and three flathead screws (2) as shown. Torque these screws to 101 N-cm (9 in-lb).

Replace Outer Cover and Rear Frame

21. Refer to Figure 1. Carefully place the spectrum analyzer on the work surface with the front frame facing down.
22. Replace the instrument outer cover by matching the grill on the bottom of the cover to the bottom of the analyzer (E401B and E4411B).
23. Replace the instrument outer cover by matching the grill on the side of the case to the fan on the A5 power supply assembly (E441A only).
24. Fit the leading edge of the case completely into the slot on the back of the front frame assembly (E4411A only).
25. The rear EMI contact grid that clips onto the rear frame can come loose. When replacing the rear frame, make sure the gasket is in the correct position.
26. Replace the rear frame assembly (6) using the four screws (5) to fasten the rear frame to the instrument. Torque these screws to 236 N-cm (21 in-lb.).

Verify Analyzer Performance (ESA Models E4401B, E4411B)

- Perform the following performance verification tests found in the *“Agilent ESA Spectrum Analyzers Calibration Guide.”*
 1. Displayed Average Noise Level
 2. Tracking Generator Absolute Amplitude and Vernier Accuracy
 3. Tracking Generator Level Flatness
 4. Tracking Generator Harmonic Spurious Outputs
 5. Tracking Generator Non-Harmonic Spurious Outputs

Verify Analyzer Performance (ESA Model E4411A)

- Perform the following performance verification tests found in the *“Agilent ESA-L1500A Spectrum Analyzer User’s and Calibration Guide.”*
 1. Tracking Generator Feedthrough
 2. Absolute Amplitude, Vernier, and Power Sweep Accuracy
 3. Tracking Generator Level Flatness
 4. Harmonic Spurious Outputs
 5. Non-Harmonic Spurious Outputs