
HP OmniBER 718

About This Book

This Quick Start Guide demonstrates the basic operation of the HP OmniBER 718, by showing you how to select displays and use them to change the instrument settings, and includes the following sections:

- Introducing the HP OmniBER Front Panel
- Introducing HP Smart Test
- Viewing Single or Multiple Windows
- Changing Instrument Settings
- Using the Pop-up Menu
- Viewing Settings on an External Monitor
- Status Alarms

Contents

Contents

Manual Conventions 4

Introduction 5

Introducing the HP OmniBER Front Panel 6

Monitoring Status Alarms 8

Introducing HP Smart Test 9

Viewing Single or Multiple Windows 11

Multiple Window Operation 11

Single Window Operation 12

Changing Instrument Settings 13

Viewing the Contents of Folders 15

Using the Pop-up Application 16

Viewing Settings on an External Monitor 18

Status Alarms 19

General Alarm Indicators 19

PDH / DS_n Alarm Indicators 19

ATM Alarm Indicators 19

Jitter Alarm Indicators 20

SDH Alarm Indicators 20

SONET Alarm Indicators 20

Manual Conventions


The conventions used in this manual to illustrate instrument keys and display information are as follows:

TRANSMIT

This is an example of a hardkey. Hardkeys (located to the right of the display) are used to give access to different sets of instrument settings, or select dedicated instrument functions. The key shown here displays the transmit settings.

PARALLEL

This is an example of a softkey. Softkeys (located below the display) are used to select instrument settings. The values associated with softkeys change as you move the display cursor from one instrument setting to another.



These are the cursor control keys. They are used to move the display cursor from one instrument setting to another.

STORED SETTINGS
SETTINGS CONTROL
FLOPPY DISK
LOGGING
REMOTE CONTROL
TIME & DATE
MISCELLANEOUS
OPTIONS
OPTION ENABLE
SELF TEST
TRIGGER OUTPUT
MODULE DEBUG
DEMO MODE
CALIBRATION
AUTO SETUP
COLOR CONTROL

This is an example of a pop-up menu. Pop-up menus are an alternative way of selecting instrument settings (instead of using softkeys). To access a pop-up menu, highlight an instrument setting, then use the **SET** key to complete the selection.



This symbol (when it appears next to settings on the display) indicates that there is a pop-up application associated with the instrument setting. To access a pop-up application, highlight the instrument setting which has this symbol, then use the **SET** key.



This symbol appears at the bottom right of the display when an optical transmit module is fitted to the instrument. The symbol's background changes from black to yellow when the optical output is switched on.

Introduction

Introduction

The HP OmniBER Communications Performance Analyzer provides all the test capability you need to fully verify the performance of today's high-capacity transmission systems and networks.




The main features of this instrument are:

- Multi-rate BER and jitter testing from 64 kb/s to 2.5 Gb/s (STM-16/OC-48)
- Concatenated payload testing up to STM-16c/OC-48c
- Full PDH/T-carrier test capability
- Measurement capabilities including protection switching tests, mixed payload generation and analysis, and pointer processing
- Fast access to key measurement tasks using HP Smart Test

Introducing the HP OmniBER Front Panel

Introducing the HP OmniBER Front Panel

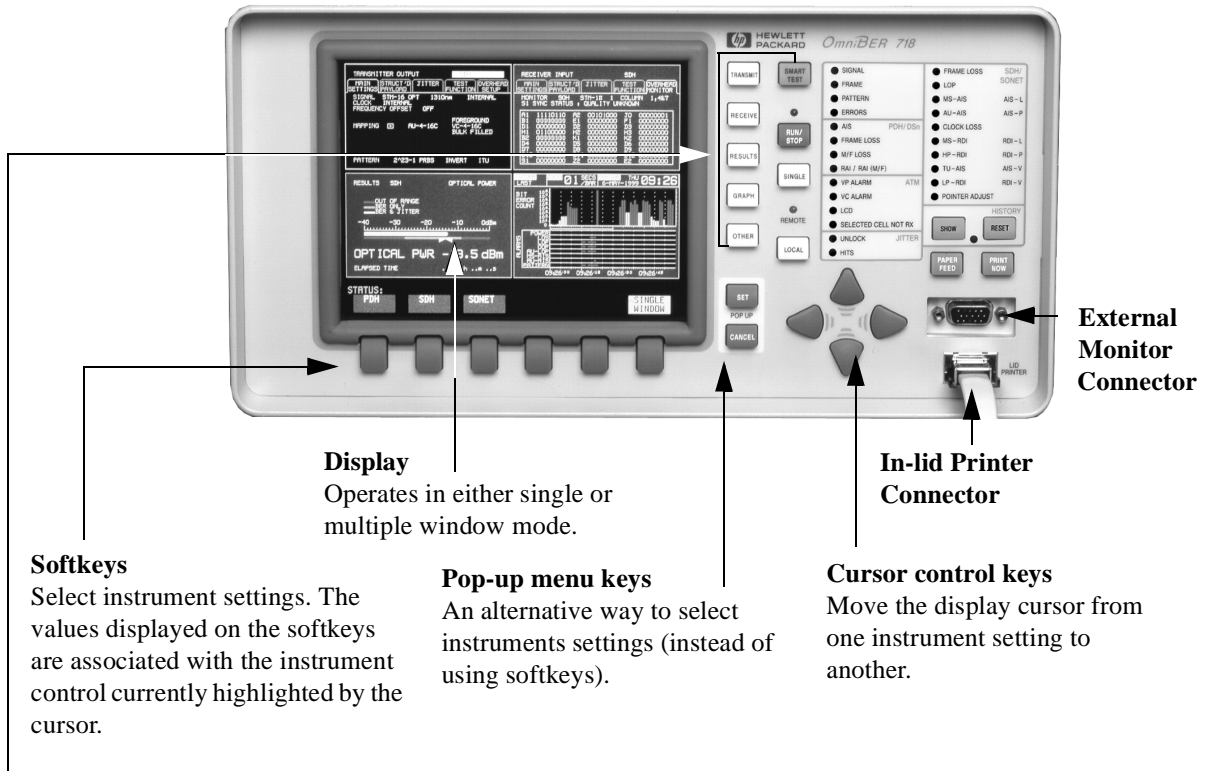

Hardkeys

SMART TEST

Press this key to access HP Smart Test settings.

TRANSMIT

Press this key to access settings associated with the transmitter.

RECEIVE

Press this key to access settings associated with the receiver.

RESULTS

Press this key to access settings associated with the test timing and graph storage, and to display measurement results.

GRAPH

Press this key to access settings associated with stored graphical results.

OTHER

Press this key to access the following instrument utilities:
Stored Settings; Settings Control; Floppy Disk, Logging (printing); Remote Control; Time & Date; Miscellaneous (settings); Options (and s/w revisions); Self Test; Trigger Output; Calibration and Color Control.


Introducing the HP OmniBER Front Panel

LOCAL

Press this key to return the instrument from Remote to Local control. The indicator above the key lights when the instrument is under Remote control.

RUN/STOP

Press this key to start a new test period or terminate the current test period. The indicator above the key lights when a test period is in progress.

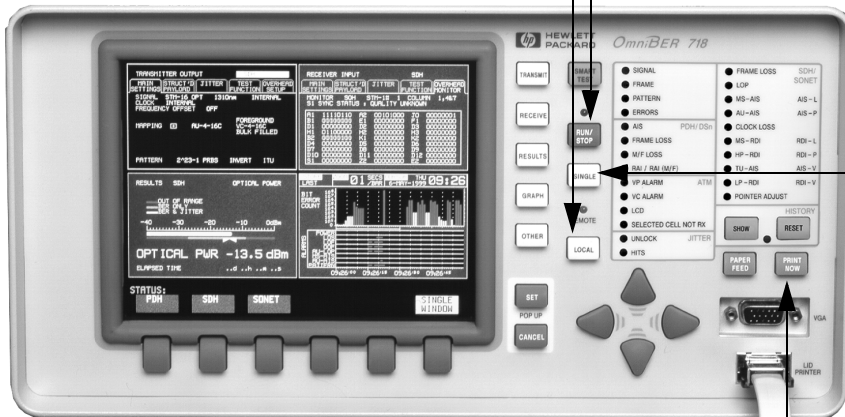

SINGLE

Press this key to add a single error to the transmitted signal. The type of error added is selected on the Error & Alarm display.

PRINT NOW

Press this key to immediately log selected results or screen dumps to the printer.

PAPER FEED

Press this key to advance the paper in the internal printer.

CAUTION


Do not press **PAPER FEED** while loading a new roll of paper in the printer. Wait until the paper is fed through the printer mechanism. A paper jam could result which would disable the printer.

Introducing the HP OmniBER Front Panel

Monitoring Status Alarms

The LED indicators provide information about the current status of the instrument's receiver. If an alarm has occurred during the current test period, the HISTORY indicator lights. The figure below shows the status indicators for the dual standard SONET/SDH option (Option 002).

These three indicators change from green to red when an alarm conditions occurs.

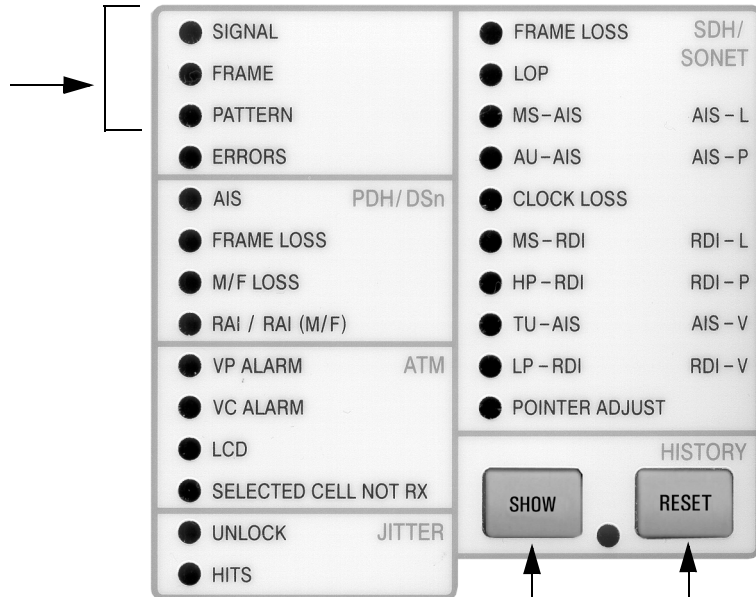

SHOW

Press and hold this key to view the alarm history. When this key is released the status indicators return to displaying the current status.

The HISTORY indicator lights when an alarm has occurred during the current test period.

RESET

Press this key to reset the HISTORY store (all lit indicators extinguish). If an alarm condition is present during the reset, then the indicators associated with that alarm will remain lit after the reset. The resetting of the HISTORY store also occurs when you start a new test period.

Introducing HP Smart Test


Introducing HP Smart Test

The HP Smart Test feature simplifies instrument operation by:

- Allowing the instrument to auto-configure on the incoming signal (Smart Setup). It will attempt to identify signal structure, and detect mixed payload signal structures.
- Allowing you to quickly access the most commonly used instrument features (Smart Tests):
 - Signal quality
 - Functional tests
 - Jitter tests
 - Settings (stored, logging, Tx/Rx coupling and trigger output enable)

To run Smart Setup:

- 1 Ensure a valid signal is connected to one of the instrument's Receive ports.
- 2 Press **SMART TEST**.

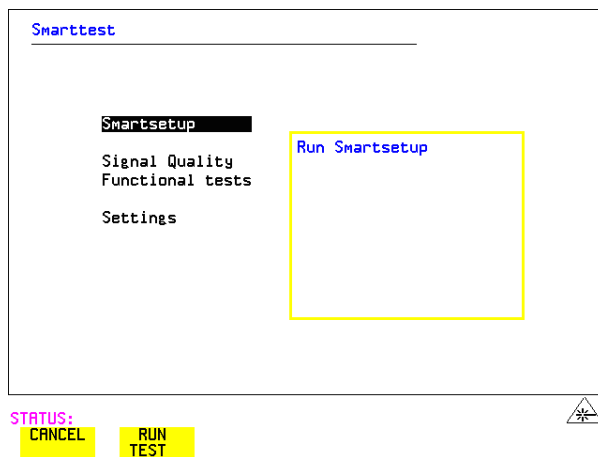


- 3 With Smartsetup highlighted, press **RUN TEST** to auto-discover information about the receive signal. Or press **CANCEL** to exit Smart Tests.

Introducing HP Smart Test

To run a Smart Test (Signal Quality - Frequency Measurement):

- 1 Ensure a valid signal is connected to one of the instrument's Receive ports.
- 2 Press **SMART TEST**.
- 3 Use the down cursor control keys to select Signal Quality.
- 4 Use the right cursor control keys to access the tests.
- 5 Use the up and down cursor control keys to select Frequency Measurement.

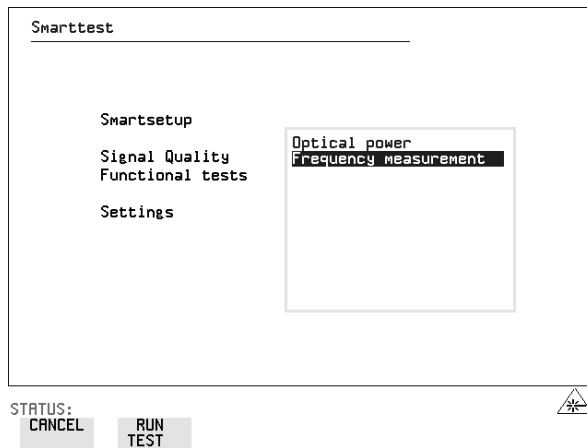

- 6 Press **RUN TEST** to display the frequency screen. Or press **CANCEL** to exit Smart Tests.

Viewing Single or Multiple Windows

Viewing Single or Multiple Windows

The instrument display can operate in either single or multiple window mode. A key at the bottom right of the display allows you to switch between modes.

Multiple Window Operation

In this mode, four windows of instrument settings appear simultaneously on the display. The active window has a black background, the others have a blue background. The active window in the figure below is the TRANSMITTER OUTPUT.

To make another window active, press either **RECEIVE**, **RESULTS**, **GRAPH** or **OTHER**. Note that, the OTHER and GRAPH windows appear at the same location (they cannot be displayed simultaneously).

The screenshot shows the instrument display with four windows. The TRANSMITTER OUTPUT window is active (black background). The other windows are RECEIVER INPUT, RESULTS, and FUNCTION. Below the windows are status indicators for PDH/DSn, SDH, and SONET. A SINGLE WINDOW key is located at the bottom right.

TRANSMITTER OUTPUT		SDH	
MAIN SETTINGS	STRUCT'D PAYLOAD	JITTER	TEST FUNCTION
SIGNAL STM-1		OVERHEAD SETUP	INTERNAL
CLOCK INTERNAL	INTERNAL		
FREQUENCY OFFSET	OFF		
MAPPING	AU-4	BACKGROUND	TU-3
34M OFFSET		34 M/s	
CHANNEL	TUG3	0 PPM	
TU PAYLOAD	UNFRAMED	1	UNSTRUCTURED
PATERN	2^23-1 PRBS	INVERT	ITU

RECEIVER INPUT		SDH	
MAIN SETTINGS	STRUCT'D PAYLOAD	TEST FUNCTION	OVERHEAD MONITOR
SIGNAL STM-1		TERMINATE	
MAPPING		AU-4	TU-3
34M OFFSET		34 M/s	
CHANNEL	TUG3	1	
TU PAYLOAD	UNFRAMED	1	UNSTRUCTURED
PATERN	2^23-1 PRBS	INVERT	ITU

RESULTS	SDH	ERROR SUMMARY
RESULT TYPE		COUNTS
FRAME	
B1 BIP	
B2 BIP	MS-REI
B3 BIP	HP-REI
HP-IEC	LP-REI
TU BIP	
B1I	
AU POINTER	0	TU POINTER 0
ELAPSED TIME	..d ..h ..m ..s	

FUNCTION	STORED SETTINGS
STORED SETTING NUMBER	0
ACTION OFF	
SETTING	0 FACTORY DEFAULT SETTINGS
1
2
3
4

STATUS:
PDH/DSn SDH SONET

SINGLE WINDOW


Press this key to select single window mode. The active window is then displayed (in this example - TRANSMITTER OUTPUT would be displayed).

Viewing Single or Multiple Windows

Single Window Operation

In this mode, only one window of instrument settings will appear on the display. The TRANSMITTER OUTPUT is shown in the figure below.

To select another window, press either **RECEIVE**, **RESULTS**, **GRAPH** or **OTHER**.

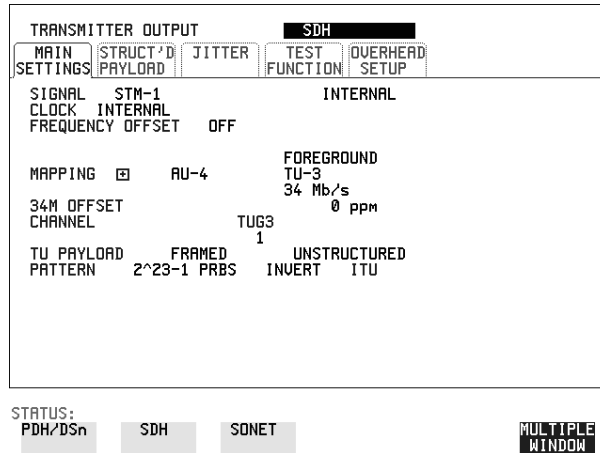


Press this key to select multiple windows.

Changing Instrument Settings

Changing Instrument Settings

Instrument settings that can be changed are displayed using white text (the cursor marks the currently selected setting field).



To change instrument settings:

- 1 Use the cursor control keys to move from one instrument setting to another. When you select a setting, the associated values are displayed on the softkey labels located at the bottom of the display.
- 2 Press the appropriate softkey to make your selection. When a setting has more than five values, press **MORE** to access the other values.

FUNCTION	LOGGING
LOGGING SETUP	DEVICE
LOGGING PORT	RS232
REMOTE CONTROL PORT	HP1B
PRINTER TYPE	HP PRINTER
SPEED	9600 BAUD
PROTOCOL	NON/NOFF

STATUS: 300 BAUD 600 BAUD 1200 BAUD 1800 BAUD MORE MULTIPLE WINDOW



Alternatively, you can use the instrument's pop-up menu feature to make your selection. With the cursor on the required setting field, press **SET** to display a pop-up menu containing the associated values. Use the up or down cursor control keys to make your selection, then press **SET**.

FUNCTION	LOGGING
LOGGING SETUP	300 BAUD
LOGGING PORT	600 BAUD
REMOTE CONTROL PORT	1200 BAUD
PRINTER TYPE	1800 BAUD
SPEED	2400 BAUD
PROTOCOL	4800 BAUD
	9600 BAUD
	NON/NOFF

STATUS: MULTIPLE WINDOW

Or press **CANCEL** to retain the current settings.

Changing Instrument Settings

In some cases when you press **SET**, instead of a pop-up menu you get a pop-up alphanumeric keypad. Examples of settings associated with the keypad are: selecting user defined Path Trace messages (in the Overhead Setup screen of the **Transmitter Output** window), or assigning a name to a stored configuration (in the Stored Settings screen of the **Other** window).

To access the pop-up keypad (to assign a name to stored a configuration):


1 Press **OTHER**.

2 Press **STORED SETTINGS**.




3 Use the up or down cursor control keys to place the cursor on the store location to be assigned a name.

4 Press **SET**.



5 Use the cursor control keys to select the character you want from the keypad, then press **SET**.

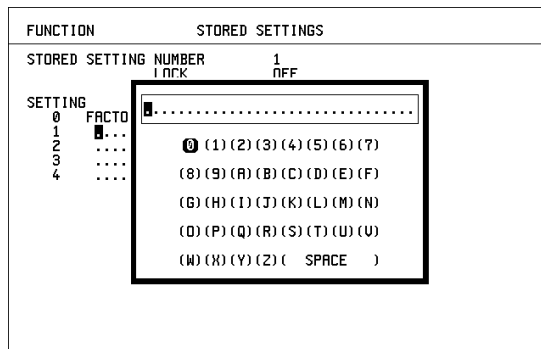

6 Repeat the previous step till you complete the name.



If you need to change any of the characters in the name, use the left and right softkeys to select the appropriate character, then repeat the previous step to select the character you want from the keypad.

7 Press **ENTER** to apply the name to the stored setting.



Changing Instrument Settings

Viewing the Contents of Folders


The instrument settings in the *Transmitter Output*, *Receiver Input*, *Results* windows are contained in folders. The figure below shows the folders in the *Transmitter Output* window.

To view the contents of the Test Function folder:

- 1 Press **TRANSMIT**.

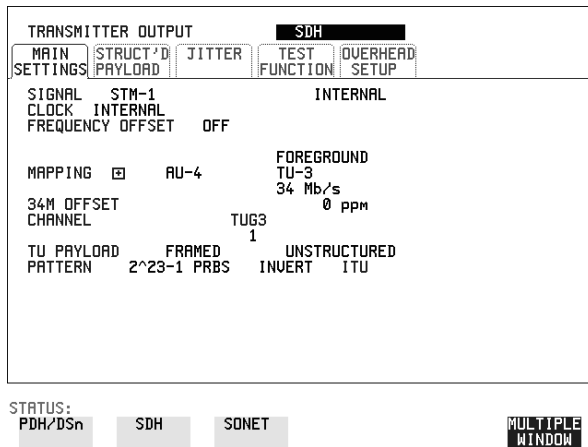

- 2 Use the down or up cursor control keys to place the cursor on the currently selected folder name. Now use the left or right cursor control keys to select the Test Function folder.

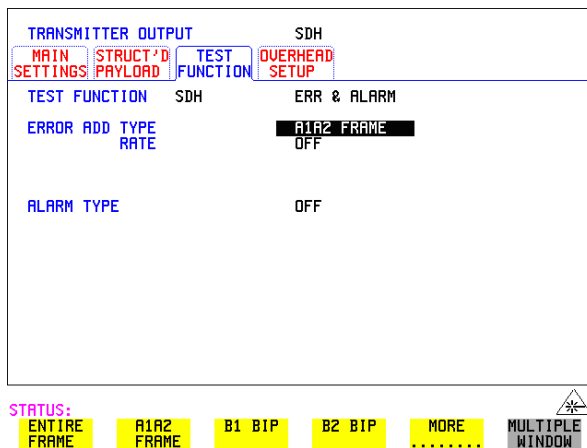

Using the Pop-up Application

Using the Pop-up Application



This symbol indicates that there is a pop-up application associated with the instrument setting.

A pop-up application is used to simplified the setting up of complex instrument configurations. In a pop-up application, instrument settings are presented to you as a pictorial or graphic “map” display.

NOTE

The modules and options fitted to your instrument determine the pop-up application that will be available to you.

To set up the SDH/SONET Payload Mapping (using the pop-up application):

- 1 Press **TRANSMIT**.

TRANSMITTER OUTPUT		SDH	
MAIN	STRUCT'D	TEST	OVERHEAD
SETTINGS	PAYLOAD	FUNCTION	SETUP
SIGNAL	STM-1	INTERNAL	
CLOCK	INTERNAL		
FREQUENCY OFFSET	OFF		
MAPPING	<input checked="" type="checkbox"/> AU-4	BACKGROUND	
		TU-3	
		34 Mb/s	
34M OFFSET			0 ppm
CHANNEL		TUG3	
		1	
TU PAYLOAD	FRAMED	STRUCTURED	
TO SET TEST SIGNAL, FIRST SELECT THE 'STRUCT'D PAYLOAD' FOLDER ABOVE.			

STATUS:

**MULTIPLE
WINDOW**

Using the Pop-up Application

- Use the cursor control keys to select the Main Settings folder, then the MAPPING settings.

TRANSMITTER OUTPUT SDH

MAIN SETTINGS
STRUCT'D PAYLOAD
TEST FUNCTION
OVERHEAD SETUP

SIGNAL STM-1 INTERNAL
CLOCK INTERNAL
FREQUENCY OFFSET OFF

MAPPING AU-4 UC-4
 140M OFFSET 140 Mb/s
0 ppm

PAYLOAD TYPE UNFRAMED UNSTRUCTURED
PATTERN 2^23-1 PRBS INVERT ITU

HINT: Press SET for popup application diagram

STATUS:

UC-4

TU-3


TU-2

TU-12

TU-11

MULTIPLE WINDOW

- Press SET to display the payload map.

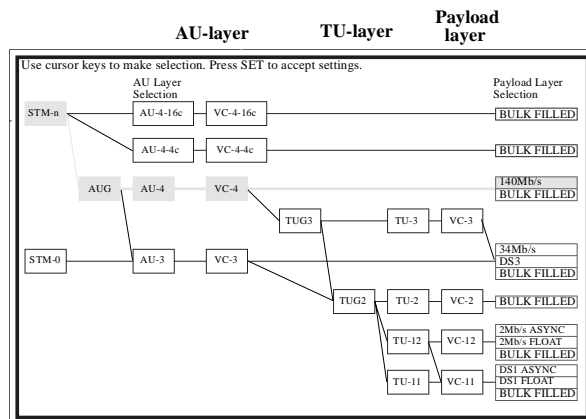

STATUS:

MULTIPLE WINDOW

To change between AU/SPE-layer, TU/VT-layer and Payload layer selections:

- Use the left and right cursor control keys.

To select the mapping you want:

- Use the up and down cursor control keys.

Viewing Settings on an External Monitor

To select the new value:

- 6 Press **SET**.
- or
- Press **CANCEL** to exit the pop-up application without making the change.

Viewing Settings on an External Monitor

For easier viewing, the instrument settings may be viewed on an external standard VGA monitor or projector.

To view instrument settings on an external monitor:

- 1 Connect the external monitor to the instruments front panel VGA connector.
- 2 Switch-on the external monitor.
- 3 The instrument settings will now appear on the external monitor.

Status Alarms

Status Alarms

General Alarm Indicators

The SIGNAL, FRAME, and PATTERN indicators are green if the signal is good, and red during an alarm condition.

SIGNAL	Green: Valid signal (level; data transitions) detected at input. Red: No data transitions detected at input.
FRAME	Green: Correct framing detected at all levels of the received signal (on the line signal plus all levels down to the selected test channel). Red: Frame alignment lost at one or more levels of the received signal.
PATTERN	Green: Correct detection of expected test pattern. Red: Expected test pattern not received.
ERRORS	A measured error has occurred. The indicator will remain lit for 100 ms.

PDH / DS_n Alarm Indicators

These are active when a PDH / DS_n signal is received

AIS	AIS detected.
FRAME LOSS	Frame alignment lost or out of alignment condition.
M/F LOSS	Multiframe alignment lost.
RAI/ RAI (M/F)	Remote alarm (x-bit or yellow alarm bit is set) or Remote Multiframe Alarm bit is set.

ATM Alarm Indicators

This group of red LED's is active when an ATM signal is received.

VP ALARM	Virtual Path AIS or FERF has been detected.
VC ALARM	Virtual Channel AIS or FERF has been detected.

Status Alarms

LCD	Loss of Cell Delineation has been detected. This occurs when 7 consecutive header errors have occurred.
SELECTED CELL NOT RX	The selected cell has not been received.

Jitter Alarm Indicators

UNLOCK	The jitter receiver has lost phase lock. Jitter measurement is suspended until lock is regained.
HITS	A jitter hit has been detected.

SDH Alarm Indicators

These are active when an SDH signal is received.

FRAME LOSS	Loss of Frame has been detected.
LOP	Loss of pointer has been detected.
MS-AIS	Multiplexer Section AIS has been detected.
AU-AIS	Path AIS has been detected.
CLOCK LOSS	The transmitter clock is not synchronized to the selected reference.
MS-RDI	Multiplexer Section RDI (FERF) has been detected.
HP-RDI	Path RDI (FERF) has been detected.
TU-AIS	TU Path AIS has been detected.
LP-RDI	TU Path RDI (FERF) has been detected.
POINTER ADJUST	A pointer change in the foreground signal has been detected.

SONET Alarm Indicators

These are active when an SONET signal is received.

FRAME LOSS	Loss of Frame or Severely Errored Frame has been detected. Status message on bottom of display states which has occurred.
LOP	Loss of Pointer has been detected.
AIS-L	Line AIS has been detected.
AIS-P	STS Path AIS has been detected.

Status Alarms

CLOCK LOSS	The transmitter clock is not synchronized to the selected reference.
RDI-L	Line RDI (FERF) has been detected.
RDI_P	Path RDI (FERF) has been detected.
AIS-V	VT Path AIS has been detected.
RDI-V	VT Path RDI (FERF) has been detected.
POINTER ADJUST	A pointer change associated with the foreground test channel has been detected (either STS pointer or VT pointer).

Index

A

AIS alarm indicator, 19
AIS-V Alarm Indicator, 21

Alarm Indicator

AIS, 19
AIS-V, 21
AU-AIS, 20
AU-LOP, 20
Clock loss, 20
Errors, 19
Frame loss, 19
HP-RDI, 20
LOF/OOF, 20
LP-RDI, 20
M/Frame loss, 19
MS-AIS, 20
MS-RDI, 20
Pattern, 19
Pointer adjust, 20, 21
RDI-L, 21
RDI-P, 21
RDI-V, 21
Remote alarm, 19
Remote M/frame alarm, 19
Signal, 19
TU-AIS, 20
TU-LOP, 20

Alarm Indicators
General, 19
PDH / DS_n, 19
SDH, 20

Alarms Reset key, 8
AU-AIS Alarm Indicator, 20

C

Cancel key, 13
changing instrument settings, 13
Clock Loss Alarm Indicator, 20
connector (for in-lid printer), 6
Cursor
Introduction to, 13
Moving, 13, 14, 15, 17
Cursor control keys, 6
cursor control keys, 13

D

Display mode (single or multiple windows), 11

Display on a monitor, 18
DS_n Alarm Indicators, 19

E

Errors, 19
Errors Alarm Indicator, 19
external monitor connector, 6
external monitor (viewing settings), 18

F

Folder
Selecting, 13
Folders, 15
Frame, 19
Frame Loss Alarm Indicator, 19
Functional Tests (Smart Test), 9

G

Graph key, 6
Graphic displays as a selection aid, 16

H

History alarms key (show), 8
History reset key, 8
HP-RDI Alarm Indicator, 20

I

Indicators
Front Panel, 19
Inlid printer connector, 6

J

Jitter Alarm Indicators, 20
Jitter Hits Alarm, 20
Jitter Tests (Smart Test), 9
Jitter Unlock alarm, 20

K

Keys
Show History, 8

L

LCD Alarm, 20
Local key, 7
LOF alarm indicator, 20
Loss Of Pointer Alarm Indicator, 20
LP-RDI Alarm Indicator, 20

M

M/Frame Loss Alarm Indicator, 19
Monitor connector, 6
Monitor, connecting, 18
MS-AIS Alarm Indicator, 20
MS-RDI Alarm Indicator, 20
multiple windows operation, 11

O

OOF alarm Indicator, 20
Other key, 6

P

Paper Feed key, 7
Pattern, 19
Pattern Alarm Indicator, 19
PDH / DS_n Alarms
AIS, 19
Frame Loss, 19
M/Frame Loss, 19
Remote Alarm, 19
Remote M/Frame Alarm, 19
PDH Alarm Indicators, 19
Pictorial displays as a selection aid, 16
Pointer Adjust Indicator, 20, 21
Pop-up Applications, 16
Pop-up keypad, 14
Pop-up menu keys, 6
Print Now key, 7

R

RDI-L Alarm Indicator, 21
RDI-P Alarm Indicator, 21
RDI-V Alarm Indicator, 21
Receive key, 6
Remote Alarm Indicator, 19
Remote M/Frame Alarm Indicator, 19
Results key, 6
Run/Stop key, 7

S

SDH Alarm Indicators, 20
SDH Alarms
AU-AIS, 20
Clock Loss, 20
HP-RDI, 20
Loss Of Pointer, 20
LP-RDI, 20

- MS-AIS, 20
- MS-RDI, 20
- Pointer Adjust, 20
- TU-AIS, 20
- SDH payload mapping with pictorial display, 16
- Selected Cell not received, 20
- Settings
 - changing with soft keys, 13
 - settings (changing), 13
- Settings (Smart Test), 9
- Show (history) Alarms key, 8
- Show History key, 8
- Signal, 10
- Signal Quality (Smart Test), 9, 10
- Single key, 7
- Single window operation, 12
- single window operation, 11
- Smart Setup, 9
- Smart Test, 6, 9
- softkeys, 6
- SONET Alarms
 - AIS-V, 21
 - Pointer Adjust, 21
 - RDI-L, 21
 - RDI-P, 21
 - RDI-V, 21
- Status Alarms, 18
- Status Indicators, 8

T

- Transmit key, 6
- TU-AIS Alarm Indicator, 20

V

- VC Alarm, 19
- VGA external monitor connector, 6
- viewing settings (external monitor), 18
- VP Alarm, 19

W

- When, 13