
HP OmniBER 718

List of Contents

General Information

Warranty	1-1
Responsibilities of the Customer	1-2
Certification	1-3
Assistance	1-3
Notice.....	1-3
Restricted Rights Legend.....	1-3
Instruments Covered By Manual.....	1-4
Storage and Shipment.....	1-4
Repackaging for Shipment	1-4
Weight and Dimensions	1-5
Safety Precautions for the Operator	1-6
Lifting/Carrying the HP OmniBER 718.....	1-6
Safety Symbols	1-7
Operators Maintenance.....	1-8
Cleaning.....	1-8
Power Supply Fuse Replacement	1-9
Removing/Inserting Modules	1-9
Statement of Compliance	1-10
Australian EMC Regulations.....	1-10
Noise Declaration (German).....	1-10
Electromagnetic Compatibility.....	1-11
Declaration of Conformity	1-12

Installation

Initial Inspection	2-1
Operating Environment	2-2
Preparation for Use.....	2-3
Power Requirements	2-3
Fuses	2-3

List of Contents

Fuse Replacement	2-3
Connecting to the Power Supply	2-4
Connecting to the Network.....	2-6
All Connectors	2-6
Electrical Interface Connectors.....	2-6
Optical Interface Connectors	2-9
Connecting Accessories.....	2-11
10 Base-T Lan Connection Radiated Emissions	2-11
General Purpose Interface Bus	2-12
Additional Precautions for Service Engineers.....	2-14
Safety Precautions	2-14
ESD Precautions	2-14
Front Panel Soft Recovery (Cold Start).....	2-16

Performance Tests

Introduction	3-1
Equipment Required	3-1
Performance Test Record	3-1
Calibration Cycle	3-1
Instrument Model and Option Configuration	3-1
Recall Default Settings	3-4
Self Test	3-5
Description.....	3-5
PDH/DSn Internal Transmitter Clock Accuracy & Offset.....	3-10
Specifications.....	3-10
Description.....	3-10
Equipment Required	3-10
Procedure	3-11
E1 (2.048Mb/s) Frequency Accuracy.....	3-11
E2 (8.448Mb/s) Frequency Accuracy.....	3-12
E3 (34.368Mb/s) Frequency Accuracy.....	3-12

List of Contents

E4 (139.264 Mb/s) Frequency Accuracy	3-13
DS1 (1.544 Mb/s) Frequency Accuracy	3-13
DS3 (44.736 Mb/s) Frequency Accuracy	3-14
PDH/DSn Transmitter Output	3-15
Specification	3-15
Description.....	3-15
Equipment Required	3-16
Procedure	3-16
Procedure - 34.368 Mb/s.....	3-19
Procedure - 8.448 Mb/s.....	3-21
Procedure - 2.048 Mb/s.....	3-23
Procedure - DSX-3	3-26
Procedure - DSX-1	3-28
PDH/DSn Receiver Equalization	3-32
Specifications	3-32
Description.....	3-32
Equipment Required	3-32
Procedure	3-33
PDH/DSn Receiver Monitor Levels	3-39
Specifications.....	3-39
Description.....	3-39
Procedure	3-40
External Mux/Demux	3-44
Specifications.....	3-44
Description.....	3-44
Equipment Required	3-44
Procedure	3-45
PDH/DSn Frequency Measurement and Looped Clock	3-54
Specifications.....	3-54
Description.....	3-54
Equipment Required	3-54
Procedure	3-54

List of Contents

SDH/SONET Transmitter Clock Accuracy	3-58
Specification	3-58
Description.....	3-58
Equipment Required	3-58
Procedure	3-58
External Clock/Data Reference Inputs & Clock Reference Output	3-59
Specifications	3-59
Description.....	3-59
Equipment Required	3-59
Procedure	3-60
SDH/SONET Frequency Offsets	3-64
Specifications.....	3-64
Description.....	3-64
Equipment Required	3-64
Procedure	3-64
STM-0/STS-1 Transmitter Output Waveshape	3-66
Specifications.....	3-66
Description.....	3-66
Equipment Required	3-66
Procedure	3-66
STM-1/STS-3 Transmitter Output Waveshape	3-70
Specifications.....	3-70
Description.....	3-70
Equipment Required	3-70
Procedure	3-70
SDH/SONET Receiver Equalization	3-75
Specifications	3-75
Description.....	3-75
Equipment Required	3-75
Procedure	3-75
Procedure	3-77
SDH/SONET Receiver Monitor Levels	3-78

List of Contents

Specifications.....	3-78
Description.....	3-78
Equipment Required	3-78
Procedure	3-78
Multirate Optical Interfaces	3-82
Specification (1310 nm Transmitter up to 622 Mb/s)	3-82
Specification (1310 nm Transmitter up to 2488.32 Mb/s)	3-82
Specification (1550 nm Transmitter up to 622 Mb/s)	3-82
Specification (1550 nm Transmitter up to 2488.32 Mb/s)	3-82
Specification (Receiver) up to 2488.32 Mb/s	3-83
Specification (Receiver) up to 622.08 Mb/s	3-83
Description.....	3-83
Equipment Required	3-84
Procedure	3-84
Performance Test Record	3-89

Terms

ETSI/ANSI Conversion and Equivalent Terms.....	4-1
--	-----

Self Test Overview

Self Tests	5-1
Overall Function Self Tests	5-1
All Tests (test time - up to 1 hour depending on options)	5-2
Specific Measurement Hardware/Function Tests.....	5-2
PDH Test (test time- approximately 20 minutes)	5-3
BER Test (test time- approximately 20 minutes)	5-4

Option Structure/Module Configuration

Introduction.....	6-1
-------------------	-----

1

General Information

Warranty

HP PRODUCT

DURATION OF WARRANTY

HP OmniBER 718

3 years

- 1** HP warrants HP hardware, accessories and supplies against defects in materials and workmanship for the period specified above. If HP receives notice of such defects during the warranty period, HP will, at its option, either repair or replace products which prove to be defective. Replacement products may be either new or like-new.
- 2** HP warrants that HP software will not fail to execute its programming instructions, for the period specified above, due to defects in material and workmanship when properly installed and used. If HP receives notice of such defects during the warranty period, HP will replace software media which does not execute its programming instructions due to such defects.
- 3** HP does not warrant that the operation of HP products will be uninterrupted or error free. If HP is unable, within a reasonable time, to repair or replace any product to a condition as warranted, customer will be entitled to a refund of the purchase price upon prompt return of the product.
- 4** HP products may contain remanufactured parts equivalent to new in performance or may have been subject to incidental use.
- 5** The warranty period begins on the date of delivery or on the date of installation if installed by HP. If customer schedules or delays HP installation more than 30 days after delivery, warranty begins on the 31st day from delivery.
- 6** Warranty does not apply to defects resulting from (a) improper or inadequate maintenance or calibration, (b) software, interfacing, parts or supplies not supplied by HP, (c) unauthorized modification or misuse, (d) operation outside of the published environmental specifications for the product, or (e) improper site preparation or maintenance.

General Information

Warranty

- 7** TO THE EXTENT ALLOWED BY LOCAL LAW, THE ABOVE WARRANTIES ARE EXCLUSIVE AND NO OTHER WARRANTY OR CONDITION, WHETHER WRITTEN OR ORAL, IS EXPRESSED OR IMPLIED AND HP SPECIFICALLY DISCLAIMS ANY IMPLIED WARRANTIES OR CONDITIONS OF MERCHANTABILITY, SATISFACTORY QUALITY, AND FITNESS FOR A PARTICULAR PURPOSE.
- 8** HP will be liable for damage to tangible property per incident up to the greater of \$300,000 or the actual amount paid for the product that is the subject of the claim, and for damages for bodily injury or death, to the extent that all such damages are determined by a court of competent jurisdiction to have been directly caused by a defective HP product.
- 9** TO THE EXTENT ALLOWED BY LOCAL LAW, THE REMEDIES IN THIS WARRANTY STATEMENT ARE CUSTOMER'S SOLE AND EXCLUSIVE REMEDIES. EXCEPT AS INDICATED ABOVE, IN NO EVENT WILL HP OR ITS SUPPLIERS BE LIABLE FOR LOSS OF DATA OR FOR DIRECT, SPECIAL, INCIDENTAL, CONSEQUENTIAL (INCLUDING LOST PROFIT OR DATA), OR OTHER DAMAGE, WHETHER BASED IN CONTRACT, TORT, OR OTHERWISE.

FOR CONSUMER TRANSACTIONS IN AUSTRALIA AND NEW ZEALAND: THE WARRANTY TERMS CONTAINED IN THIS STATEMENT, EXCEPT TO THE EXTENT LAWFULLY PERMITTED, DO NOT EXCLUDE, RESTRICT OR MODIFY AND ARE IN ADDITION TO THE MANDATORY STATUTORY RIGHTS APPLICABLE TO THE SALE OF THIS PRODUCT TO YOU.

Responsibilities of the Customer

The customer shall provide:

- 1** Access to the products during the specified periods of coverage to perform maintenance.
- 2** Adequate working space around the products for servicing by Hewlett-Packard personnel.
- 3** Access to and use of all information and facilities determined necessary by Hewlett-Packard to service and/or maintain the products. (Insofar as these items may contain proprietary or classified information, the customer shall assume full responsibility for safeguarding and protection from wrongful use.

General Information

Warranty

- 4** Routine operator maintenance and cleaning as specified in the Hewlett-Packard Operating and Service Manuals.
- 5** Consumables such as paper, disks, magnetic tapes, ribbons, inks, pens, gases, solvents, columns, syringes, lamps, septa, needles, filters, frits, fuses, seals, detector flow cell windows, etc.

Certification

Hewlett-Packard Company certifies that this product met its published specifications at the time of shipment from the factory. Hewlett-Packard further certifies that its calibration measurements are traceable to the United States National Bureau of Standards, to the extent allowed by the Bureau's calibration facility and to the calibration facilities of other International Standards Organization members!

Assistance

Product maintenance agreements and other customer assistance agreements are available for Hewlett-Packard products.

Notice

The information contained in this document is subject to change without notice.

Hewlett-Packard shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance or use of this material.

This document contains proprietary information which is protected by copyright. All rights are reserved. No part of this document may be photocopied or reproduced without the prior written consent of the manufacturer, Hewlett-Packard Ltd.

Restricted Rights Legend

Use, duplication, or disclosure by the government is subject to restrictions as set forth in subdivision (b)(3)(ii) of the Rights in Technical Data and Computer Software clause at 52.227-7013. Hewlett-Packard Company; 3000 Hanover Street; Palo Alto, California 94304.

Instruments Covered By Manual

Attached to the rear panel of the instrument is a serial number plate. The serial number plate has a two letter reference denoting country of origin (GB = Great Britain) and an eight digit serial number. The serial number is unique to each instrument and should be quoted in all correspondence with Hewlett-Packard, especially when ordering replacement parts. Refer to Chapter 6 for instrument options covered.



Serial Number Plate

Storage and Shipment

The instrument may be stored or shipped in environments within the following limits:

Temperature	-20° C to +70° C -15° C to +50° C with lid printer
Altitude	Up to 4,600 meters (15,000 feet)

The instrument should also be protected from temperature extremes which could cause condensation within the instrument.

Repackaging for Shipment

Tagging for Service. If the instrument is being returned to Hewlett-Packard for service, please complete a repair tag and attach it to the instrument.

General Information

Weight and Dimensions

Original Packaging. Containers and materials identical to those used in factory packaging are available from Hewlett-Packard offices. If the instrument is being returned to Hewlett-Packard for servicing, attach a tag indicating the type of service required, return address, model number, and full serial number. Mark the container FRAGILE to ensure careful handling. In any correspondence, refer to the instrument by model number and full serial number.

Other Packaging. The following general instructions should be followed when repackaging with commercially available materials:

- Wrap instrument in heavy paper or plastic. If the instrument is being shipped to Hewlett-Packard, attach a tag indicating the type of service required, return address, model number and full serial number.
- Use a strong shipping container. A double wall carton made of 350 pound test material is adequate.
- Use a layer of shock absorbing material 70 to 100 mm (3 to 4 inch) thick, around all sides of the instrument to provide firm cushioning and prevent movement inside the container. Protect the Front Panel controls and Rear Panel connectors with cardboard.
- Seal shipping container securely.
- Mark shipping container FRAGILE to ensure careful handling.
- In any correspondence, refer to instrument by model number and full serial number.

Weight and Dimensions

Weight: 18 kg (40 lb) fully loaded

Dimensions: 190mm (7.5in) high, 340mm (14in) wide, 420mm (17in) deep (including cover).

Safety Precautions for the Operator

The following general safety precautions must be observed during all phases of operation, service, and repair of this instrument. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the instrument. Hewlett-Packard Company assumes no liability for the customer's failure to comply with these requirements.

In particular, the operator should note the following safety information:

- “Safety Symbols” on page 1-7
- “Connecting to the Power Supply” on page 2-4
- “Operating Environment” on page 2-2
- “Fuse Replacement” on page 2-3
- “Operators Maintenance” on page 1-8
- “Lifting/Carrying the HP OmniBER 718” on page 1-6

DO NOT operate damaged equipment: Whenever it is possible that the safety protection features built into this product have been impaired, either through physical damage, excessive moisture, or any other reason, **REMOVE POWER** and do not use the product until safe operation can be verified by service-trained personnel. If necessary, return the product to a Hewlett-Packard Sales and Service Office for service and repair to ensure the safety features are maintained.

Lifting/Carrying the HP OmniBER 718

Before attempting to lift or carry the instrument consider the following basic lifting techniques to help avoid personal injury.

Using both arms to lift instrument.

- Reach for the instrument - bend your knees and waist, and keep your back straight.
- GRASP the instrument firmly.
- LIFT with your legs.
- KEEP your shoulders level.

General Information

Safety Precautions for the Operator

Safety Symbols


The following symbols on the instrument and in the manual indicate precautions which must be taken to maintain safe operation of the instrument



The Instruction Documentation Symbol. The product is marked with this symbol when it is necessary for the user to refer to the instructions in the supplied documentation.



Indicates the field wiring terminal that must be connected to earth ground before operating the equipment - protects against electrical shock in case of fault.



Frame or chassis ground terminal - typically connects to the equipment's metal frame.



Alternating current (AC)



Direct current (DC)



Indicates hazardous voltages

WARNING

Warning denotes a hazard. It calls attention to a procedure, which if not correctly performed or adhered to could result in injury or loss of life. Do not proceed beyond a warning note until the indicated conditions are fully understood and met.

CAUTION



Caution denotes a hazard. It calls attention to a procedure, which if not correctly performed or adhered to could result in damage to or destruction of the instrument. Do not proceed beyond a caution note until the indicated conditions are fully understood and met.



Indicates that a laser is fitted. The user must refer to the manual for specific Warning or Caution information to avoid personal injury or damage to the product.

Operators Maintenance

WARNING

NO OPERATOR SERVICEABLE PARTS INSIDE. REFER SERVICING TO QUALIFIED PERSONNEL. TO PREVENT ELECTRICAL SHOCK DO NOT REMOVE COVERS.

Maintenance appropriate for the operator is:

- Cabinet cleaning
- Optical Connector Cleaning
- Power supply fuse replacement
- Ensure ventilating fan cover is clean.

Cleaning

Instrument Cleaning

Clean the cabinet using a dry cloth only.

Optical Connector Cleaning

It is recommended that the optical connectors be cleaned at regular intervals using the following materials:

Description	HP Part Number
Blow Brush	9300-1131
Isopropyl Alcohol	8500-5344
Lens Cleaning Paper	9300-0761
Adhesive Tape Kit	15475-68701

CAUTION

Do not insert any tool or object into the IN or OUT ports of the instrument as damage to or contamination of the optical fibre may result.

General Information

Operators Maintenance

- 1** Recall Default settings (STORED SETTINGS 0) and remove the power from the HP OmniBER 718.
- 2** Remove the adapters from the IN and OUT ports. Use an 11 mm spanner to slacken the nut securing the adapter. On re-assembly tighten the nut using a torque spanner to 1.5 Nm.
- 3** Using the blow brush with the brush removed blow through the ferrule of the standard flexible connector and the adapter.

CAUTION

If the optical fibre of the fixed connector requires further cleaning this entails disassembly of the module which should only be carried out by suitably trained service personnel.

- 4** Apply some isopropyl alcohol to a piece of the cleaning paper and clean the barrel of the adapter. Using a new piece of cleaning paper, clean the face of the adapter. Repeat this operation, using a new piece of cleaning paper each time.
- 5** Lightly press the adhesive side of the tape provided against the front of the adapter, then remove it quickly - repeat twice. This removes any particles of cleaning paper which may be present.
- 6** Replace the adapters on the flexible connector.

Power Supply Fuse Replacement

See "Fuse Replacement" on page 2-3.

Removing/Inserting Modules

Modules should only be removed or inserted by trained personnel.

Statement of Compliance

This instrument has been designed and tested in accordance with IEC Publication 1010-1 + A1:1992 Safety requirements for Electrical Equipment for Measurement, Control and Laboratory Use, and has been supplied in a safe condition. The instruction documentation contains information and warnings which must be followed by the user to ensure safe operation and to maintain the instrument in a safe condition.



The CE mark shows that the product complies with all relevant European legal Directives.

ISM 1-A

This is a symbol of an Industrial Scientific and Medical Group 1 Class A product.



The CSA mark is a registered trademark of the Canadian Standards Association.

Australian EMC Regulations



The C-Tick mark is a registered trademark of the Spectrum Management Agency of Australia. This signifies compliance with the Australian EMC Framework Regulations under the terms of the Radiocommunications Act of 1992.

Noise Declaration (German)

LpA<70dB

am Arbeitsplatz (operator position)

normaler Betrieb (normal position)

nach DIN 45635 pt.19 (per ISO 7779)

Electromagnetic Compatibility

This product has been designed to meet the protection requirements of the European Communities Electromagnetic Compatibility (EMC) directives:

EN55011:1991 (Group 1, Class A)

EN50082-1:1992

- IEC 1000-4-2 (1995) ESD

- IEC 1000-4-3 (1995) Radiated Susceptibility

- IEC 1000-4-4 (1995) EFT

In order to preserve the EMC performance of the product, any cable which becomes worn or damaged must be replaced with the same type and specification.

General Information
Declaration of Conformity

Declaration of Conformity according to ISO/IEC Guide 22 and EN45014		
Manufacturer's Name:	Hewlett-Packard Ltd.	
Manufacturer's Address:	Telecomms Networks Test Division South Queensferry West Lothian, EH30 9TG Scotland, United Kingdom	
Declares that the product		
Product Name:	HP OmniBER 718 Communications Performance Analyzer	
Model Number:	HP 37718A	
Product Options:	This declaration covers all options of the above product as detailed in TCF A-5951-9852-01	
Conforms with the protection requirements of European Council Directive 89/336/EEC on the approximation of the laws of the member states relating to electromagnetic compatibility, against EMC test specifications EN 55011:1991 (Group 1, Class A) and EN 50082-1:1992.		
As Detailed in:	Electromagnetic Compatibility (EMC) Technical Construction File (TCF) No. A-5951-9852-01	
Assessed by:	DTI Appointed Competent Body EMC Test Centre, GEC-Marconi Avionics Ltd., Maxwell Building, Donibristle Industrial Park, Hillend, Dunfermline KY11 9LB Scotland, United Kingdom	
Technical Report Number:6893/2200/CBR, dated 21 August 1997		
Supplementary Information:		
The product conforms to the following safety standards:		
EN 61010-1(1993) IEC 61010-1(1990) +A1(1992) +A2(1995) CSA-C22.2 No. 1010.1-93 CFR Ch.1 1040.10 EN 60825-1(1994) / IEC 825-1(1993)		
The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC, and carries the CE marking accordingly.		
<i>South Queensferry, Scotland</i>	<i>28 May 1999</i>	
<i>Location</i>	<i>Date</i>	<i>W.R. Pearson / Quality Manager</i>

Europe Contact:
Your Local Hewlett-Packard Sales and Service Office or Hewlett-Packard GmbH, Department 2Q / Standards
Europe
Herrenberger Strasse 130, D7030 Boblingen (Fax: +49-7031-143143)

General Information
Declaration of Conformity

Declaration of Conformity according to ISO/IEC Guide 22 and EN45014		
Manufacturer's Name:	Hewlett-Packard Ltd.	
Manufacturer's Address:	Telecomms Networks Test Division South Queensferry West Lothian, EH30 9TG Scotland, United Kingdom	
Declares that the product		
Product Name:	HP OmniBER 718 Communications Performance Analyzer	
Model Number:	HP 37718B	
Product Options:	This declaration covers all options of the above product as detailed in TCF A-5951-9852-01	
Conforms with the protection requirements of European Council Directive 89/336/EEC on the approximation of the laws of the member states relating to electromagnetic compatibility, against EMC test specifications EN 55011:1991 (Group 1, Class A) and EN 50082-1:1992 .		
As Detailed in:	Electromagnetic Compatibility (EMC) Technical Construction File (TCF) No. A-5951-9852-01	
Assessed by:	DTI Appointed Competent Body EMC Test Centre, GEC-Marconi Avionics Ltd., Maxwell Building, Donibristle Industrial Park, Hillend, Dunfermline KY11 9LB Scotland, United Kingdom	
Technical Report Number:6893/2200/CBR, dated 21 August 1997		
Supplementary Information:		
The product conforms to the following safety standards:		
EN 61010-1(1993) IEC 61010-1(1990) +A1(1992) +A2(1995) CSA-C22.2 No. 1010.1-93 CFR Ch.1 1040.10 EN 60825-1(1994) / IEC 825-1(1993)		
The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC, and carries the CE marking accordingly.		
<i>South Queensferry, Scotland</i>	<i>30 July 1999</i>	
<i>Location</i>	<i>Date</i>	<i>W.R. Pearson / Quality Manager</i>

Europe Contact:
Your Local Hewlett-Packard Sales and Service Office or Hewlett-Packard GmbH, Department 2Q / Standards
Europe
Herrenberger Strasse 130, D7030 Boblingen (Fax: +49-7031-143143)

General Information
Declaration of Conformity

Declaration of Conformity according to ISO/IEC Guide 22 and EN45014		
Manufacturer's Name:	Hewlett-Packard Ltd.	
Manufacturer's Address:	Telecomms Networks Test Division South Queensferry West Lothian, EH30 9TG Scotland, United Kingdom	
Declares that the product		
Product Name:	HP OmniBER 718 Communications Performance Analyzer	
Model Number:	HP 37718C	
Product Options:	This declaration covers all options of the above product as detailed in TCF A-5951-9852-01	
Conforms with the protection requirements of European Council Directive 89/336/EEC on the approximation of the laws of the member states relating to electromagnetic compatibility, against EMC test specifications EN 55011:1991 (Group 1, Class A) and EN 50082-1:1992 .		
As Detailed in:	Electromagnetic Compatibility (EMC) Technical Construction File (TCF) No. A-5951-9852-01	
Assessed by:	DTI Appointed Competent Body EMC Test Centre, GEC-Marconi Avionics Ltd., Maxwell Building, Donibristle Industrial Park, Hillend, Dunfermline KY11 9LB Scotland, United Kingdom	
Technical Report Number:6893/2200/CBR, dated 21 August 1997		
Supplementary Information:		
The product conforms to the following safety standards:		
EN 61010-1(1993) IEC 61010-1(1990) +A1(1992) +A2(1995) CSA-C22.2 No. 1010.1-93 CFR Ch.1 1040.10 EN 60825-1(1994) / IEC 825-1(1993)		
The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC, and carries the CE marking accordingly.		
<i>South Queensferry, Scotland</i>	<i>30 July 1999</i>	
<i>Location</i>	<i>Date</i>	<i>W.R. Pearson / Quality Manager</i>

Europe Contact:
Your Local Hewlett-Packard Sales and Service Office or Hewlett-Packard GmbH, Department 2Q / Standards
Europe
Herrenberger Strasse 130, D7030 Boblingen (Fax: +49-7031-143143)

2

Installation

Initial Inspection

WARNING

TO AVOID HAZARDOUS ELECTRICAL SHOCK, DO NOT PERFORM ELECTRICAL TESTS WHEN THERE ARE SIGNS OF SHIPPING DAMAGE TO ANY PORTION OF THE OUTER ENCLOSURE (COVERS, PANELS, METERS).

Inspect the shipping container for damage. If the shipping container or cushioning material is damaged, it should be kept until the contents of the shipment have been checked for completeness and the instrument has been checked both mechanically and electrically. Procedures for checking electrical operation are given in Chapter 3. If the contents of the shipment are incomplete, if there is mechanical damage or defect, notify the nearest Hewlett-Packard Office. If the instrument does not pass the electrical performance tests given in Chapter 3, notify the nearest Hewlett-Packard office. If the shipping container is also damaged, or the cushioning material shows signs of stress, notify the carrier as well as the nearest Hewlett-Packard office. Keep the shipping materials for the carrier's inspection. The Hewlett-Packard office will arrange for repair or replacement without waiting for claim settlement.

Operating Environment

This instrument is designed for Indoor use only.

DO NOT operate the product in an explosive atmosphere or in the presence of flammable gasses or fumes.

This instrument may be operated in environments within the following limits:

Temperature: 0°C to +45°C
+5°C to +40°C for Jitter operation
+5°C to +35°C with lid printer

Altitude up to 3050 m (10,000 ft)

Humidity up to 95% relative humidity to 40°C, but it should be protected from temperature extremes which may cause condensation.

To ensure adequate cooling do not obstruct air vents in the instrument cabinet. Do not for example operate the instrument if it is standing on its rear feet, as air vents may be obstructed by floor covering.

CAUTION

This instrument is designed for use in Installation Category II and Pollution Degree 2 per IEC 610.0-1 and 644 respectively.

CAUTION

VENTILATION REQUIREMENTS: When installing the instrument in a cabinet, the convection into and out of the instrument must not be restricted. If the total power dissipated in the cabinet is greater than 800 watts, then forced convection must be used.

Preparation for Use

WARNING

FOR CONTINUED PROTECTION AGAINST FIRE HAZARD REPLACE FUSE ONLY WITH SAME TYPE AND RATINGS (see “Fuses” on page 2-3).

WARNING

If this instrument is not used as specified, the protection provided by the equipment could be impaired. This instrument must be used in a normal condition only (in which all means for protection are intact).

Power Requirements



The HP OmniBER 718 Communications Performance Analyzer requires a power source of 100 V to 240 V ac at a frequency between 47 Hz and 63 Hz (nominal).

Total power consumption is 450 VA (maximum).

The fuse rating for the power source is given in the following table.

Fuses

Line Voltage	Fuse Rating	HP Part Number
100 V to 240 V	5 A Timed, 250 V	2110-1120

Fuse Replacement

Only the ac line fuse located at the rear of the instrument may be replaced by the operator.

WARNING

ALL OTHER FUSE REPLACEMENT SHOULD ONLY BE CARRIED OUT BY SUITABLY TRAINED SERVICE PERSONNEL AWARE OF THE HAZARDS INVOLVED.

WARNING

BEFORE REMOVING THE FUSE, THE AC LINE POWER CORD SHOULD BE DISCONNECTED FROM THE POWER SOURCE AND THE OTHER END DISCONNECTED FROM THE INSTRUMENT.

Installation
Preparation for Use

WARNING

ONLY USE A FUSE OF THE CORRECT RATING AS LISTED IN “Fuses” on page 2-3. DO NOT use repaired fuses or short-circuited fuseholders: For continued protection against fire, replace the line fuse(s) only with fuse(s) of the same voltage and current rating and type.

The fuse is removed by inserting a suitable flat bladed tool into the slot in the fuse cap and turning counter-clockwise. The cap and the fuse can then be removed and the fuse changed for another of the correct rating. The fuse rating and HP part number are listed in “Fuses” on page 2-3.

Connecting to the Power Supply

WARNING

This is a Safety Class I instrument (provided with a protective earthing ground, incorporated in the powercord). The mains plug shall only be inserted in a socket outlet provided with a protective earth contact. Any interruption of the protective conductor inside or outside of the instrument is likely to make the instrument dangerous. Intentional interruption is prohibited.

CAUTION

Before switching on this instrument, make sure that the line supply voltage is in the specified ranges. Range selection is automatic.

Installation
Preparation for Use

Power Cord

WARNING

TO AVOID THE POSSIBILITY OF INJURY OR DEATH, THE FOLLOWING PRECAUTIONS MUST BE FOLLOWED BEFORE THE INSTRUMENT IS SWITCHED ON:-

WARNING

(a) Note that the protection provided by grounding the instrument cabinet may be lost if any power cable other than the three-pronged type is used to couple the ac line voltage to the instrument.

WARNING







(b) If this instrument is to be energized via an auto-transformer to reduce or increase the line voltage, make sure that the common terminal is connected to the neutral pole of the power source.

WARNING

(c) The power cable plug shall only be inserted into a socket outlet provided with a protective ground contact. The protective action must not be negated by the use of an extension cord without a protective conductor (grounding).

The power cord supplied with each instrument varies with the country of destination. The following figure illustrates the standard power plug and cord configurations that are commonly used. The part number shown beneath each plug is the part number of the appropriate power cord and plug. If the appropriate power cord is not included with the instrument notify the nearest Hewlett-Packard office and a replacement will be provided.

Power Cord Configurations and Part Numbers

						
8120-2104	8120-1369	8120-1689	8120-1351	8120-1378 US 8120-4753 JAP	8120-2956	8120-4211


Connecting to the Network

The network connectors are located on the modules at the side of the instrument. The connections available depend on the options fitted to your instrument.

Before Connecting, note the Warning and Caution information given.

All Connectors

CAUTION



When connecting or disconnecting, ensure that you are grounded or, make contact with the metal surface of the Mainframe with your free hand to bring you, the module, and the mainframe to the same static potential.

Modules remain susceptible to ESD damage while the module is installed in the Mainframe

Additional ESD information is required when servicing see “Additional Precautions for Service Engineers” on page 2-14.

Electrical Interface Connectors

RECEIVER **2,8,34,140 IN**

PDH receiver input interface. Allows the connection of 75 Ω unbalanced data signals (all rates) and 120 Ω balanced data signals at 2 Mb/s.

TRANSMIT **2,8,34,140 OUT**

PDH transmitter output interface. Provides 75 Ω unbalanced data output (all rates) and 120 Ω balanced data output at 2 Mb/s

DS3, 2Mb/s, **34Mb/s 75 Ω IN**

PDH/DSn receiver input interface. Allows the connection of 75 Ω unbalanced DS3, 2 Mb/s and 34.368 Mb/s data signals.

DS3, 2Mb/s, **34Mb/s 75 Ω OUT**

PDH / DSn transmitter output interface. Provides 75 Ω unbalanced DS3, 2 MB/s and 34 Mb/s data output. A “keep alive” signal is output when the transmit signal is SDH/SONET.

DS1 100 Ω , **2Mb/s 120 Ω IN**

PDH / DS1 receiver input interface. Allows the connection of 100 Ω balanced DS1 and 120 Ω balanced 2 Mb/s data signals.

Installation

Connecting to the Network

DS1 100 Ω, 2Mb/s 120 Ω OUT

PDH / DS1 transmitter output interface. Provides 100 Ω balanced DS1 and 120 Ω balanced 2 Mb/s data signals. A “keep alive” signal is output when the transmit signal is SDH/SONET.

52/155 Mb/s DATA IN

SDH/SONET receiver input interface. Allows the connection of 75 Ω unbalanced STM 0/1, STS 1/3 electrical signals.

52/155 Mb/s DATA OUT

SDH/SONET transmitter output interface. Provides a 75 Ω unbalanced STM 0/1, STS 1/3 electrical output.

64k REF IN 1.5M REF IN 2M REF IN

These ports allow connection of timing reference signals. Note, unused ports must not have a signal present.

REF OUT

Provides a 2 MHz reference Clock Output.

MUX

Allows the insertion of an external 2 Mb/s tributary into the transmitted payload.

MUX DS1 100 Ω

Allows an externally supplied DS1 signal to be inserted in any or all timeslot(s) of a DS3 signal. In conjunction with the SDH/SONET module a DS1 signal can be inserted into a VT1.5 or TU-11.

MUX 2 Mb/s 75 Ω

Allows an externally supplied 2.048 Mb/s signal to be inserted in any or all timeslot(s) of a 34 Mb/s signal. In conjunction with the SDH module a 2.048 Mb/s signal can be inserted into a TU-12.

DEMUX DS1 100 Ω

Allows a DS1 signal to be dropped from any timeslot of a DS3 signal. In conjunction with the SDH/SONET module this port allows the demultiplexing of a DS1 signal carried in a VT1.5

DEMUX 2 Mb/s 75 Ω

Allows a 2.048 Mb/s signal to be dropped from any timeslot of an 8.448 Mb/s, 34.368 Mb/s or 139.264 Mb/s signal.

Installation

Connecting to the Network

CLOCK TRIGGER Reference SDH/SONET clock trigger output 51 MHz; nominal +/- 400 mV into 50 ohms.

DCC Allows the Drop and Insert of Regenerator Section (192 kb/s) and Multiplexer Section (576 kb/s) Data Communication Channels (DCC).

The following connections are available:

Pin Number	Connection
1	Shield Ground
2	Data input for Tx(-)
3	Tx Clock
4	Data Output from Rx(-)
5	NC
6	Rx Clock(-)
7	NC
8	Signal Ground
9	Data Input for Tx(+)
10	Tx Clock(+)
11	Data output from Rx(+)
12	NC
13	Rx Clock(+)
14	NC
15	NC

**PROTECTED
MONITOR POINT
INPUT** 52/155/622 Mb/s (NRZ); Line Code NRZ; Level nominal 1 V Pk-Pk into 50 ohms;
SMA connector.

Installation
Connecting to the Network

Optical Interface Connectors

For your protection, review all laser information given in this manual before installing or using the instrument.

WARNING

To prevent personal injury, avoid use that may be hazardous to others, and maintain the module in a safe condition. Ensure the information given below is reviewed before operating the module.

Laser Product Classification

All optical modules are classified as Class I (non-hazardous) laser product in the USA which complies with the United States Food and Drug Administration (FDA) Standard 21 CFR Ch.1 1040.10, and are classified as Class 1 (non-hazardous) laser products in Europe which complies with EN 60825-1 (1994).

To avoid hazardous exposure to laser radiation, it is recommended that the following practices are observed during system operation:

- **ALWAYS DEACTIVATE THE LASER BEFORE CONNECTING OR DISCONNECTING OPTICAL CABLES.**
- When connecting or disconnecting optical cables between the module and device-under-test, observe the connection sequences given below.
 - Connecting:** Connect the optical cable to the input of the device-under-test **before** connecting to the module's *Optical Out* connector.
 - Disconnecting:** Disconnect the optical cable from the module's *Optical Out* connector **before** disconnecting from the device-under-test. Always fit the fibre optic connector dust caps over the laser aperture.
- NEVER examine or stare into the open end of a broken, severed, or disconnected optical cable when it is connected to the module's *Optical Out* connector.
- Arrange for service-trained personnel, who are aware of the hazards involved, to repair optical cables.

Installation

Connecting to the Network

CAUTION

1. Use of controls or adjustments or performance of procedures other than those specified herein may result in hazardous radiation exposure.
 2. Always fit the fibre optic connector dust caps on each connector when not in use. Before connection is made, *always* clean the connector ferrule tip with acetone or alcohol and a cotton swab. Dry the connector with compressed air. Failure to maintain cleanliness of connectors is liable to cause excessive insertion loss.
-

Laser Warning Symbols

The front panel of the optical module has the following label:

CLASS 1 LASER PRODUCT

NOTE

CLASS 1 LASER PRODUCT translates as follows:

Finnish - LUOKAN 1 LASERLAITE

Finnish/Swedish - KLASSE 1 LASER APPARAT

This label indicates that the radiant energy present in this instrument is non-hazardous.

OPTICAL IN

Allows connection of an optical signal, wavelength 1200 to 1600 nm, at a maximum power level of -8 dBm (HP 37718A) or -3 dBm (HP 37718B/C). **NEVER EXCEED +3 dBm.**

Accepts STM-0, STM-1 and STM-4. Also accepts SONET signals OC-1, OC-3, OC-12, and OC-48 depending on the model and options fitted.

OPTICAL OUT

Provides an STM-0, STM-1, STM-4 or STM-16 optical signal (OC-1, OC-3, OC-12 or OC-48 SONET signals) at wavelength 1280 to 1335nm, and/or 1480 to 1580 nm, at a nominal power level of +1 dBm depending on model and options.

Cleaning Optical Connectors

See “Optical Connector Cleaning” on page 1-8

Connecting Accessories

LID Provides the output for the option 602 printer which is fitted in the cover (LID) of the instrument.

VGA Provides the output for a display monitor.

HANDSET Allows connection of a telephone handset for communication across the network.

Printer
HP-IB (GPIB),
RS232,
PARALLEL ONLY

External printer connection details are given in the Users Guide.
The port selected for external printer use is not available for remote control.

Remote Control
HP-IB (GPIB),
RS232,
10 BASE -T

Remote control connection is given in the Remote Control Manual.
The port selected for remote control use is not available for an external printer.

10 Base-T Lan Connection Radiated Emissions

To ensure compliance with EN 55011 (1991) a category 5, FTP patch lead, RJ45 cable should be used to connect the LAN port on the processor module marked "10 Base-T".

Installation
Connecting Accessories

General Purpose Interface Bus

The HP OmniBER 718 Communications Performance Analyzer (Option 601) is connected to the GPIB by means of an appropriate GPIB cable. The GPIB interconnecting cables available are listed in the following table.

GPIB Interconnecting Cables

Length	Accessory Number
1 meter	HP 10833A
2 meters	HP 10833B
4 meters	HP 10833C
0.5 meter	HP 10833D

To achieve interface design performance standards, restrictions are placed on the GPIB system cable lengths. These restrictions allow the bus interface electronics to maintain correct line voltage levels and timing relationships.


When connecting an GPIB system the following rules should be observed:

The total GPIB cable length used must be less than or equal to 20 meters (65.6 feet).

The total GPIB cable length used must be less than or equal to 2 meters (6 feet) × the total number of devices connected to the bus.

A standard GPIB connector is provided on the instrument. The connections are shown in the following figure. The mating connector part number is HP 1251-0293 or Amphenol 57-30240.

Installation
Connecting Accessories

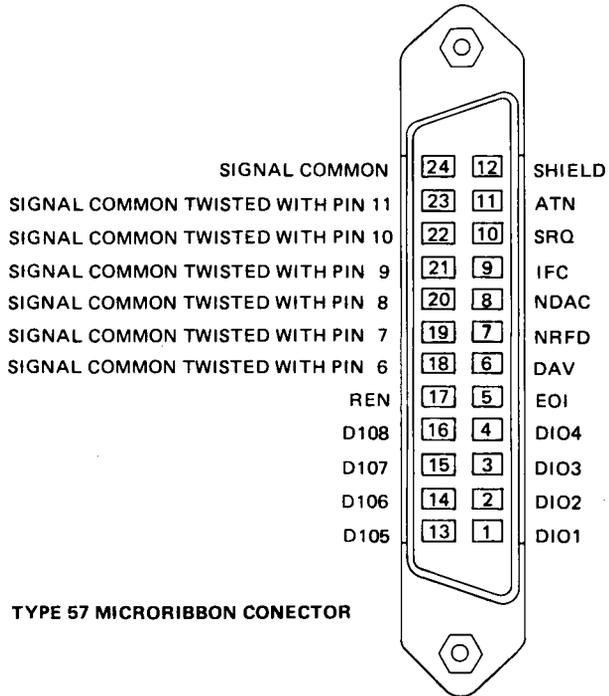

GPIB Address Selection

The HP OmniBER 718 (Option 601) GPIB address is accessed on the OTHER display under the REMOTE CONTROL function.

The address can be set to any value between 0 and 30 inclusive.

Additional Precautions for Service Engineers

Safety Precautions


DO NOT substitute parts or modify equipment: Because of the danger of introducing additional hazards, do not install substitute parts or perform any unauthorized modification to the product. Return the product to a Hewlett-Packard Sales and Service Office for service and repair to ensure the safety features are maintained.

DO NOT service or adjust alone: Under certain conditions, dangerous voltages may exist even with the equipment switched off. To avoid dangerous electrical shock, service personnel must not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

Review “Safety Precautions for the Operator” on page 1-6.

ESD Precautions

CAUTION



When making connections to the modules, review “Connecting to the Network” on page 2-6.

The module contains components sensitive to electrostatic discharge. To prevent component damage, carefully follow the handling precautions presented below.

The smallest static voltage most people can feel is about 3500 volts. It takes less than one tenth of that (about 300 volts) to destroy or severely damage static sensitive circuits. Often, static damage does not immediately cause a malfunction but significantly reduces the component’s life. Adhering to the following precautions will reduce the risk of static discharge damage.

- Keep the module in its conductive storage box when not installed in the Main-frame. Save the box for future storage of the module.
- Before handling the module, select a work area where potential static sources are minimized. Avoid working in carpeted areas and non-conductive chairs. Keep body movement to a minimum. Hewlett-Packard recommends that you use a controlled static workstation.
- Handle the module by its front-panel. Avoid touching any components or edge

Installation

Additional Precautions for Service Engineers

connectors. When you install the module, keep one hand in contact with the protective bag as you pick up the module with your other hand. Then, before installing the module, ensure that you are grounded or make contact with the metal surface of the Mainframe with your free hand to bring you, the module, and the mainframe to the same static potential. **This also applies whenever you connect/disconnect cables on the front-panel.**

Front Panel Soft Recovery (Cold Start)

Use the following procedure if you need to perform a front panel soft recovery (i.e. cold start) of the instrument.

Soft Recovery Procedure

- 7** Switch off the instrument.
- 8** On the instrument front panel - press and hold softkeys 0 and 4 simultaneously (the softkeys immediately below the display; key 0 is on the extreme left).
- 9** Power up the HP OmniBER 718 while holding the softkeys pressed.
- 10** When the LOS LED has flashed OFF and then ON again, the keys can be released.
- 11** The LOS LED will flash OFF/ON again several times (7), followed by an audible 'beep' and the display indicating 'Initializing Instrument'.
- 12** Once the initiations is complete the display will indicate:
'Firmware Revision Update'
'Default settings assumed'
Hit any key to attempt restart'
- 13** Hit any key, then wait approximately 10 seconds. The instrument should return to its default settings and normal operation.

3

Performance Tests

Introduction

The procedures given in this Section, test the HP OmniBER 718 performance using the Specifications provided, as performance standards. Tests are intended to be performed in the recommended order for a full instrument calibration check. Tests can be run individually, however it will be assumed that any preceding test would meet specifications.

Equipment Required

Equipment required for the Performance Tests is given in this Chapter. Any equipment which meets or exceeds the critical specification of the equipment listed, may be substituted. Recommended models are those typically used in HP Service Centers. Alternative models are also listed.

Performance Test Record

The results of the Performance Tests may be recorded on the Test Records at the end of this Chapter. The Performance Test Record lists all the tested specifications and the acceptable limits. The results recorded at incoming inspection may be used for comparison during periodic maintenance, troubleshooting or after repair or adjustment.

Calibration Cycle

This instrument requires periodic verification of performance. Depending on use and environmental conditions, the instrument should be checked approximately once every 2 years, using these Performance Tests.

Instrument Model and Option Configuration

Please refer to Chapter 6 and the instrument Specifications for information on option configuration.

Performance Tests

Introduction

Figure 3-1 Recommended Test Equipment

Instrument	Critical Specification	Recommended Model
Oscilloscope	400 MHz Bandwidth, 1 M Ω Input Termination Telecom mask measurement capability.	HP 54520A opt 001 or HP 54810A opt 001
Frequency Synthesizer	75 Ω Output, Sinewave to 80 MHz, Amplitude to 3 V pk-pk at 10 kHz, 1 Hz resolution	HP 3335A opt 001 or HP 3325B & HP 8657A with 50/75 Ω matching pad
Signal Generator	Sinewave 700 kHz to 170 MHz, Amplitude 500 mV	HP 8657A
Frequency Counter	Range 0 to 200 MHz, 2 channels with accuracy <0.1ppm. (Ratio Mode)	HP 5325A opt 010 or HP 53181A opt 001
Spectrum Analyzer**	Frequency >2.5 Gb/s. Resolution bandwidth 10 Hz.	HP 8560E
Optical Coupler**	1310 and 1510 nm. 10/90% output.	HP 15477C
Optical Power Meter and Sensor Module	Range -8 dBm to -15 dBm, Wavelength 1270-1560 nm	HP 8153A and HP 81536A
Lightwave Converter	Wavelength 1300 to 1560 nm, Conversion Gain >300 volts/watt, Frequency Response < 3 dB down at 1 GHz.	HP 11982A opt 012
Optical Attenuator	Wavelength 1200 - 1600 nm, Range 0 - 30 dB	HP 8157A or HP 8156A opt 100
FC/PC Optical Interface Connector	Unique	HP 81000FI (Qty 4)
Optical Cables	Unique	HP 11871A (Qty 2)
PDH Structured Test Set	Unique	HP OmniBER 718, HP OmniBER 719 or HP 37717C opt UKJ
64 kb/s Clock Generator	64 kb/s ternary clock.	HP 37732A
75 Ω Attenuator Kit	0 to 200 MHz 3, 6, 10, 20 dB fixed attenuator pads	HP 86213A
Cable Simulator #E1	75 Ω coaxial cable 6 dB loss at 1 MHz	8120-0049 (120 m)*
Cable Simulator #E2	75 Ω coaxial cable 6 dB loss at 4 MHz	8120-0049 (80 m)*
Cable Simulator #E3	75 Ω coaxial cable 12 dB loss at 17 MHz	8120-0049 (120 m)*
Cable Simulator #E4	75 Ω coaxial cable 12 dB loss at 70 MHz	8120-0049 (80 m)*
Cable Simulator #E1-M	75 Ω coaxial cable 3 dB loss at 1 MHz	8120-0049 (60 m)*

Performance Tests
Introduction

Figure 3-1 Recommended Test Equipment, continued

Instrument	Critical Specification	Recommended Model
Cable Simulator #E2-M	75Ω coaxial cable 3 dB loss at 4 MHz	8120-0049 (40 m)*
Cable Simulator #E3-M	75Ω coaxial cable 6 dB loss at 17 MHz	8120-0049 (60 m)*
Cable Simulator #E4-M	75Ω coaxial cable 6 dB loss at 70 MHz	8120-0049 (40 m)*
Cable Simulator #DS1	75Ω coaxial cable. Equivalent to 655 feet ABAM cable.	8120-0049 (80m)*
Cable Simulator #DS3	75Ω coaxial cable. Equivalent to 450 feet of 728A cable	8120-0049 (55m)*
Cable Simulator STM-0/STS-1	75Ω coaxial cable 6 dB loss at 26 MHz	8120-0049 (50 m)*
Cable Simulator STM-1/STS-3	75Ω coaxial cable 12 dB loss at 78 MHz	8120-0049 (75 m)*
75Ω Termination	0 to 200 MHz	HP 15522-80010
T Connector	BNC to Dual BNC	HP 1250-0781
Adaptor	SMA to BNC	1250-1787 (Qty 2)
Adaptor	Type N to BNC	HP 1250-1534 (Qty 2)
Adaptor	Type N to N	HP 1250-1528 (Qty 2)
Balanced/Unbalanced Converter	110Ω balanced: 75Ω Unbalanced (nominal)	HP 15508B (Qty 2)
Blocking Capacitor	0.18uF 200V	HP 10240B

* Note: Cable lengths quoted are typical for the half bit rate loss. Ideally, cables should be trimmed to correct length/loss by measuring with a Network Analyzer.

** Note: Spectrum Analyzer/Optical Coupler are only required for HP OmniBER Jitter options.

Self Test Loopback Cables and Accessories

HP E4545A 3m fibre optic cable FC/CP connectors. (supplied accessory)

HP E4546A FC/CP 15 dB attenuator. (supplied accessory)

HP 15525A 75 ohm BNC, 3 off.

HP 15512A Siemens 3 pin

HP 15670A Bantam 110 ohm, 2 off.

DCC 15 pin loopback plug - see figure in DCC Test.

Formatted floppy disk.


Performance Tests

Introduction

Recall Default Settings

The Performance Tests require the HP OmniBER 718 to be set to a pre-defined (default) state at the beginning of each test.

- 1 Using **OTHER**, display softkeys, **↓** **↑** **→** and **←** set up the **OTHER** **STORED SETTINGS** display as shown opposite

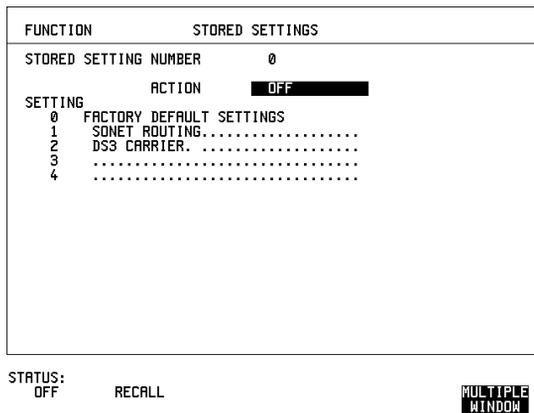


- 2 Press **RECALL** to recall the instrument default settings. The instrument display will blank for a few seconds while the settings are recalled and the status display will indicate stored settings number 0 recalled.

Self Test

Self Test

Description

Before carrying out the performance tests run Self Test to ascertain the integrity of the HP OmniBER 718. These tests take at least 1 hour to complete depending on the options fitted. Alternatively you can run Confidence Tests which only takes 2 to 3 minutes to complete. This is not a full verification but performs BER measurements with internal and external loopbacks fitted.

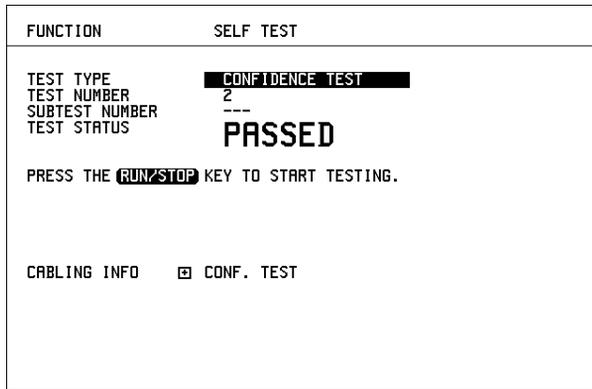

STATUS:
ALL TESTS CPU TESTS CONF. TESTS PDH TESTS MORE MULTIPLE WINDOW

Run Confidence TESTS

- 1 Choose TEST TYPE **CONF. TESTS** on the **OTHER** **SELF TEST** display.

CAUTION

Safety precaution, care and connection cleanliness are essential to avoid optical signal degradation or damage. see Operators Maintenance in chapter 1 and see Optical Interface Connectors in chapter 2 if in doubt.
The use of air-gap attenuators is not recommended.
Failure to attenuate the optical signal could result in damage to the optical receiver.

Performance Tests

Self Test

NOTE

If the Optical Interface is a Dual Wavelength Option the **1550 nm** IN and OUT ports are not connected at this stage and can be tested later.

If any or all of these connections are not made the HP OmniBER 718 will FAIL Self Test.

- 2** Make the loopback connections listed below:
Connect the 15 dB optical attenuator provided at the Optical OUT and then connect the attenuator output to Optical IN using the optical cable supplied with your instrument.
Connect Multirate Analyser IN to OUT.
Connect Transmit module 75 Ω OUT to Receive module 75 Ω IN.
Connect Transmit module 100/120 Ω OUT to Receive module 100/120 Ω IN.
- 3** Press **RUN/STOP** to activate the Self Test. TEST STATUS RUNNING will be displayed.
The information pertaining to TEST TYPE, TEST NUMBER and SUBTEST NUMBER will change as the Self Test progresses.
If the HP OmniBER 718 is functioning correctly, after a time of 2 to 3 minutes, TEST STATUS PASSED is displayed.
If TEST STATUS [FAIL nnn] is displayed, check the displayed error information and check loopback connections are correct. Repeat the test and if the problem persists contact your local HP representative. See Chapter 5 for information.

NOTE

Each individual self test requires unique loopback connections. To obtain a list of the connections required move the highlighted cursor to CABLING INFO and press **SET**. The Loopbacks list will appear on the display. Also refer to Chapter 5 for Self Test connection information.

Performance Tests

Self Test

FUNCTION	SELF TEST
TEST TYPE	PDH TESTS
TEST NUMBER	3
SUBTEST NUMBER	---
TEST STATUS	RFADV

PDH SELFTEST - CABLING INFORMATION

PAYLOAD MODULE CONNECTIONS :

- CONNECT PDH OUT TO PDH IN (UNBALANCED DS3, 210k/s, 341k/s)
- CONNECT PDH OUT TO PDH IN (BALANCED 210k/s)
- CONNECT MUX TO DEMUX (BALANCED DS1)
- CONNECT MUX TO DEMUX (UNBALANCED 210k/s)

STATUS:

**MULTIPLE
WINDOW**

Run ALL TESTS

- 1 Choose TEST TYPE **ALL TESTS** on the **OTHER SELF TEST** display.
- 2 Insert a formatted disk into the instrument disk drive.
- 3 Make the loopback connections listed below:
Connect the 15 dB optical attenuator provided, to Optical OUT and connect the attenuator output to Optical IN.
Connect Multirate Analyser IN to OUT.
Connect Transmit module 75 Ω OUT to Receive module 75 Ω IN.
Connect Transmit module 100/120 Ω OUT to Receive module 100/120 Ω IN.
Connect Transmit module 75 Ω MUX to Receive module 75 Ω DEMUX.
Connect Transmit module 100/120 Ω MUX to Receive module 100/120 Ω DEMUX.
- 4 Press **RUN/STOP** to activate the Self Test. TEST STATUS RUNNING will be displayed.
The information pertaining to TEST TYPE, TEST NUMBER and SUBTEST NUMBER will change as the Self Test progresses.
If the HP OmniBER 718 is functioning correctly, after a time of at least 1 hour, TEST STATUS PASSED is displayed.
If TEST STATUS [FAIL nnn] is displayed, check the displayed error information and check loopback connections are correct. Repeat the test and if the problem persists contact your local HP representative. See Chapter 5 for information.

Performance Tests

Self Test

FUNCTION	SELF TEST
TEST TYPE	ALL TESTS
TEST NUMBER	0
SUBTEST NUMBER	---
TEST STATUS	READY
PRESS THE RUN/STOP KEY TO START TESTING.	
CABLING INFO	<input type="checkbox"/> ALL

STATUS: ALL TESTS CPU TESTS CONF. TESTS PDH TESTS MORE **MULTIPLE WINDOW**

1550 nm Dual Wavelength Tests:

If a Dual Wavelength Optical Interface is fitted, repeat the CONFIDENCE test with 1550 nm selected.


- 1 Select 1550 nm OPTICS wavelength
- 2 Connect 1550 nm OUT to IN via 15 dB Optical Attenuator. Ensure the attenuator is inserted in the OUT port.
- 3 Run the test.

Performance Tests

Self Test

DCC Port Tests:

- 1 Select BER TESTS
- 2 Make the following connections at the Multirate Analyzer DCC port.

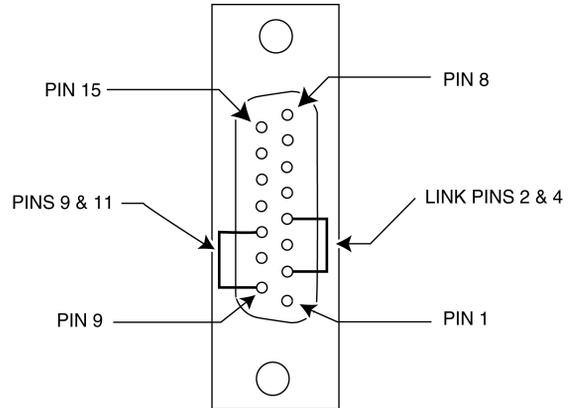

- 3 Run the BER TESTS.

PDH/DSn Internal Transmitter Clock Accuracy & Offset

Specifications

Rate	Frequency
E4	139.264 MHz \pm 4.5 ppm
E3	34.368 MHz \pm 4.5 ppm
E2	8.448 MHz \pm 4.5 ppm
E1	2.048 MHz \pm 4.5 ppm
DS1	1.544 MHz \pm 4.5 ppm
DS3	44.736 MHz \pm 4.5 ppm

Description

This test verifies that the PDH transmit data rates are within limits. These limits assume the instrument is within the calibration cycle. The Frequency Offset capability (deviation from Standard Bit Rate) is also checked.

For E1 to E4 a Frequency Counter connected to the PDH/DSn Signal Out port measures the data rate on an “all ones” pattern. This gives an indirect measure of the internal transmitter clock frequency as the data is clocked by the internal clock oscillator. Because the Frequency Counter triggers from the positive pulses only, the frequency count will, for Ternary signals E1, E2 & E3, be half the selected data rate. For DS-1 and DS-3 the Frequency Counter is connected to the CLOCK OUT port.

Equipment Required

Frequency Counter	: HP 5335A Option 010
75Ω Termination	: HP 15522-80010
T Connector	: HP 1250-0781

Performance Tests

PDH/DSn Internal Transmitter Clock Accuracy & Offset

Procedure

- 1 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on Page 3-4.
- 2 Connect the 75Ω OUT port of the PDH/DSn module to the Frequency Counter. Terminate the Frequency Counter input in 75Ω (use the T connector).
- 3 Set the **TRANSMIT** display as shown opposite

TRANSMITTER OUTPUT		PDH/DSn
MAIN SETTINGS	STRUCT'D SETTINGS	TEST FUNCTION
SIGNAL		2 Mb/s
CLOCK SYNC		INTERNAL
TERMINATION		75Ω UNBAL
LINE CODE		HDB3
FREQUENCY OFFSET		OFF
PAYLOAD TYPE	UNFRAMED	UNSTRUCTURED
PATTERN		ALL ONES

STATUS:
2²³-1 PRBS ALL ZEROS ALL ONES 1010 MORE **MULTIPLE WINDOW**

NOTE

When changing the PDH Rate or Offset value the VCXO takes time to settle. As a consequence the frequency counter reading will not stabilize until “*VCXO OUTPUT BIT RATE SETTLING*” clears from the STATUS line of the display.

E1 (2.048Mb/s) Frequency Accuracy

- 4 Adjust the Frequency Counter ATEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 1023995 Hz and 1024005 Hz.
- 5 Select FREQUENCY OFFSET [+50PPM].
- 6 Adjust the Frequency Counter ATEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 1024046.5 Hz and 1024055.5 Hz.

Performance Tests

PDH/DSn Internal Transmitter Clock Accuracy & Offset

- 7 Select FREQUENCY OFFSET [-50PPM].
- 8 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 1023944 Hz and 1023953 Hz.

E2 (8.448Mb/s) Frequency Accuracy

- 9 Select SIGNAL [8Mb/s]; PATTERN [ALL 1's] on the **TRANSMIT** display.
- 10 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 4223981 Hz and 4224019 Hz.
- 11 Select FREQUENCY OFFSET [+30PPM].
- 12 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 4224107.5 Hz and 4224145.7 Hz.
- 13 Select FREQUENCY OFFSET [-30PPM].
- 14 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 4223854 Hz and 4223892 Hz.

E3 (34.368Mb/s) Frequency Accuracy

- 15 Select SIGNAL [34Mb/s] PATTERN [ALL 1's] on the **TRANSMIT** display.
- 16 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 17183922.7 Hz and 17184077.4 Hz.
- 17 Select FREQUENCY OFFSET [+20PPM]
- 18 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 17184266 and 17184421 Hz.
- 19 Select FREQUENCY OFFSET [-20PPM]
- 20 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 17183579 Hz and 17183734 Hz.

Performance Tests

PDH/DSn Internal Transmitter Clock Accuracy & Offset

- 21 Select FREQUENCY OFFSET [USER OFFSET] [+100PPM]
- 22 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 17185641 Hz and 17185796 Hz.
- 23 Select FREQUENCY OFFSET [USER OFFSET] [-100PPM]
- 24 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 17182205 Hz and 17182359 Hz.

NOTE

Please note if Options 012 is fitted the E4 rate is generated from the 75Ω OUT port of the E4 Clock Card which is situated next to the PDH/DSn module.

E4 (139.264 Mb/s) Frequency Accuracy

- 25 Select SIGNAL [140 Mb/s] PATTERN [ALL 1's] on the **TRANSMIT** display.
- 26 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 69631686.5 Hz and 69632318.5 Hz.
- 27 Select FREQUENCY OFFSET [+15PPM].
- 28 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 69632731 Hz and 69633358 Hz.
- 29 Select FREQUENCY OFFSET [-15PPM].
- 30 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 69630642 Hz and 69631269 Hz.

DS1 (1.544 Mb/s) Frequency Accuracy

- 31 Connect the CLOCK OUT port of the PDH/DSn module to the Frequency Counter.
- 32 Select SIGNAL [DS1 1.5 Mb/s] on the **TRANSMIT** display.
- 33 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 1543993 Hz and 1544007 Hz.
- 34 Select FREQUENCY OFFSET [+32PPM]

Performance Tests

PDH/DSn Internal Transmitter Clock Accuracy & Offset

- 35 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 1544042 Hz and 1544056 Hz.
- 36 Select FREQUENCY OFFSET [-32PPM]
- 37 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 1543944 Hz and 1543958 Hz.

DS3 (44.736 Mb/s) Frequency Accuracy

- 38 Connect the CLOCK OUT port of the PDH/DSn module to the Frequency Counter.
- 39 Select SIGNAL [DS3] on the **TRANSMIT** display.
- 40 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 44735799 Hz and 44736201 Hz.
- 41 Select FREQUENCY OFFSET [+20PPM]
- 42 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 44736693 Hz and 44737096 Hz.
- 43 Select FREQUENCY OFFSET [-20PPM]
- 44 Adjust the Frequency Counter ATTEN and Trigger Level to obtain a stable reading and ensure that the frequency counter reading is between 44734904 Hz and 44735307 Hz.
- 45 Disconnect all the test equipment.

PDH/DSn Transmitter Output

Specification

Rate	Level	Waveshape
DSX-1	2.4 V - 3.6 V	Fits mask T1.102-1993
DS1-LO	As DSX-1 with 655' ABAM Cable	
DS3-HI	0.36 V - 0.85 V	
DSX-3	560 mV pk (nominal)	Fits mask T1.102-1993
DS3-900	330 mV pk (nominal)	
E1 Balanced	3.00 V (nominal)	As per ITU rec G703
E1 Unbalanced	2.37 V (nominal)	As per ITU rec G703
E2 Unbalanced	2.37 V (nominal)	As per ITU rec G703
E3 Unbalanced	1.0 V (nominal)	As per ITU rec G703
E4 Unbalanced	1.0 V \pm 0.1 V	As per ITU rec G703

Description

This test ensures the transmitter output level and pulse shape meet the required specifications at all PDH/DSn rates. The Transmitter output is connected to an Oscilloscope and the waveshape compared with the predefined masks stored in the Oscilloscope memory. The signal levels are also measured using the Oscilloscope.

Performance Tests

PDH/DSn Transmitter Output

Equipment Required

Oscilloscope	: HP 54520A Option 001
110Ω/75Ω Balanced to Unbalanced Converter	: HP 15508B
75Ω Termination	: HP 15522-80010

Procedure

NOTE


This performance test is written using the HP 54520A Oscilloscope with Option 001 - Telecom Masks Application. If any other Oscilloscope is used the keystrokes given in this procedure will not apply. The Positive pulse masks are contained in the ROOT directory of the Telecom Mask Application Disk and the Negative pulse masks are in the INV_MASK directory.

Installing the Telecom Masks Option

- 1 Insert the Disk containing the Telecom Mask into the Oscilloscope Disk Drive.
- 2 Press SHIFT (Blue Key) DISK
- 3 Press **DIRECTORY** softkey then **ROOT DIRECTORY** softkey

139.264 Mb/s - All 1's Pulse

- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4.
- 2 Set the **TRANSMIT** display as shown below.

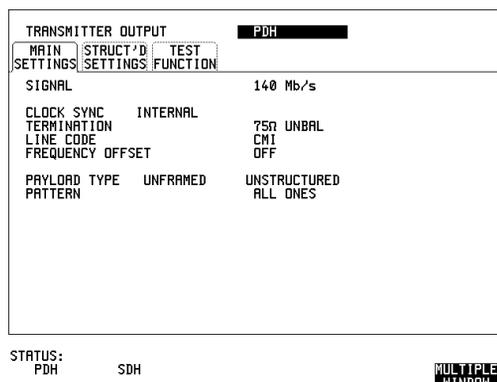

Performance Tests

PDH/DSn Transmitter Output

- 3 Connect the 139Mb/s 75Ω OUT port to the Oscilloscope CHAN 1, terminate in 75Ω.
- 4 Select CHAN 1 on the Oscilloscope and set to 1 MΩ input impedance.

Load the Telecom Mask

- 5 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 139BIN1 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 6 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 7 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 8 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 900 mV-1.1V Pk-Pk.

All 0's Pulse

- 9 Select PATTERN [ALL 0's] on the **TRANSMIT** display.

Performance Tests

PDH/DSn Transmitter Output

Load the Telecom Mask

- 10 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 139BIN0 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 11 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 12 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 13 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 900 mV-1.1V Pk-Pk.
- 14 Select PATTERN to [ALL 0's] on the **TRANSMIT** display.
- 15 On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey
- 16 Repeat steps 5 to 13 to check pulses against Inverted masks.


Performance Tests

PDH/DSn Transmitter Output

Procedure - 34.368 Mb/s

Positive Pulse

- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4.
- 2 Set the **TRANSMIT** display as shown opposite.

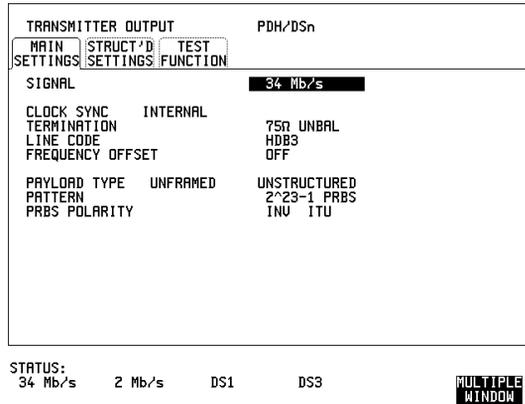

- 3 Connect the PDH/DSn 75Ω OUT port to the Oscilloscope CHAN 1, terminate in 75Ω.
- 4 Select CHAN 1 on the Oscilloscope and set to 1 MΩ input impedance.

Load the Telecom Mask

- 5 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 34MG703 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 6 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8

Performance Tests

PDH/DSn Transmitter Output

- b/ DEFINE MEAS
- c/ **COMPARE** softkey
- d/ **TEST ON** softkey
- e/ **M1M2** softkey
- f/ **AFTER FAIL CONTINUE** softkey
- g/ RUN

- 7 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 8 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 1.0 Volt.

Negative Pulse

- 9 On the Oscilloscope, use the following key sequence to access the inverted mask.
- a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey

Load the Telecom Mask

- 10 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
- a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 34MG703 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 11 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
- a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey

Performance Tests

PDH/DSn Transmitter Output

- d/ **TEST ON** softkey
- e/ **M1M2** softkey
- f/ **AFTER FAIL CONTINUE** softkey
- g/ RUN

12 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope

NOTE


It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

13 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 1.0 Volt.

Procedure - 8.448 Mb/s

Positive Pulse

- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4.
- 2 Set the **TRANSMIT** display as shown opposite.

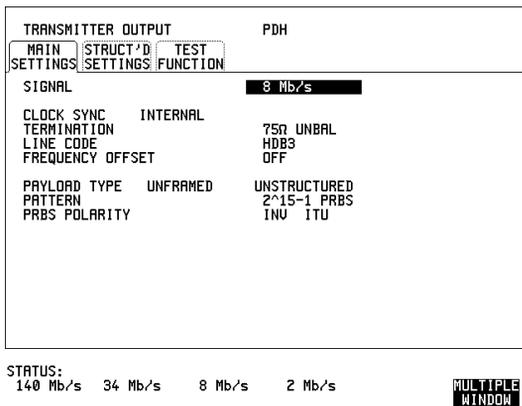

- 3 Connect the PDH/DSn 75Ω OUT port to the Oscilloscope CHAN 1, terminate in 75Ω.
- 4 Select CHAN 1 on the Oscilloscope and set to 1 MΩ input impedance.

Performance Tests

PDH/DSn Transmitter Output

Load the Telecom Mask

- 5 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 8MG703 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 6 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 7 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 8 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 2.37 Volts.

Negative Pulse

- 9 On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey

Performance Tests

PDH/DSn Transmitter Output

Load the Telecom Mask

- 10 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 8MG703 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 11 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN

- 12 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 13 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 2.37 Volts.

Procedure - 2.048 Mb/s


Positive Pulse

- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4.

Performance Tests

PDH/DSn Transmitter Output

- Set the **TRANSMIT** display as shown below.

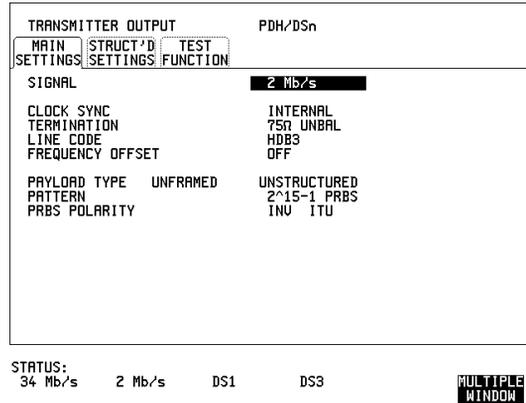

- Connect the PDH/DSn 75Ω OUT port to the Oscilloscope CHAN 1, terminate in 75Ω.
- Select CHAN 1 on the Oscilloscope and set to 1 MΩ input impedance.

Load the Telecom Mask

- On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - SHIFT (Blue Key) APPLICATION.
 - TELECOM MASK/MASK** softkey.
 - Use ENTRY/MEASURE control to select DS_1E in the highlighted MSK FILES window.
 - LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - RECALL 8
 - DEFINE MEAS
 - COMPARE** softkey
 - TEST ON** softkey
 - M1M2** softkey
 - AFTER FAIL CONTINUE** softkey
 - RUN

Performance Tests

PDH/DSn Transmitter Output

- 7 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 8 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 2.37 Volts.

Negative Pulse

- 9 On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey

Load the Telecom Mask

- 10 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select DS_1E in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 11 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 12 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

Performance Tests

PDH/DSn Transmitter Output

NOTE


It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 13 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 2.37 Volts.

Procedure - DSX-3

Positive Pulse

- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4.
- 2 Set the **TRANSMIT** display as shown below.

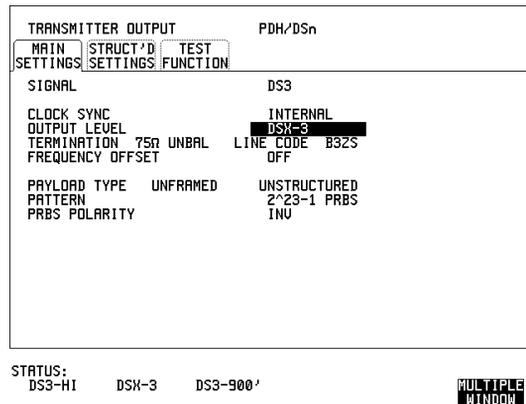

- 3 Connect the PDH/DSn 75Ω OUT port to the Oscilloscope CHAN 1, terminate in 75Ω.
- 4 Select CHAN 1 on the Oscilloscope and set to 1 MΩ input impedance.

Load the Telecom Mask

- 5 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.

Performance Tests

PDH/DSn Transmitter Output

- b/ **TELECOM MASK/MASK** softkey.
- c/ Use ENTRY/MEASURE control to select DS3_92 in the highlighted MSK FILES window.
- d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 6 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 7 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to select **MASK** softkey and **MASK AUTO** / **MASK ALIGN** or visibly fit the waveform to the mask by adjusting the Oscilloscope vertical gain/ position and horizontal delay to obtain a PASS on the Mask.

- 8 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 360 mV and 850 mV.

Negative Pulse

- 9 On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey

Load the Telecom Mask

- 10 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.

Performance Tests

PDH/DSn Transmitter Output

- c/ Use ENTRY/MEASURE control to select DS3_92 in the highlighted MSK FILES window.
- d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 11 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 12 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to select **MASK** and **MASK AUTO** / **MASK ALIGN** to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical gain/position and horizontal delay to obtain a PASS on the Mask.

- 13 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 360 mV and 850 mV.
- 14 Set the **TRANSMIT** signal to HIGH and check that the peak pulse amplitude is approximately 0.9V.
- 15 Set the **TRANSMIT** signal to LOW and check that the peak pulse amplitude is approximately 0.3V.

Procedure - DSX-1


Positive Pulse

- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4.
- 2 Connect the DSn 100Ω OUT port to the Oscilloscope via the HP 15508B Balanced to unbalanced Converter and terminate in 75Ω at the Oscilloscope input.
- 3 Select the Transmitter Output page.

Performance Tests

PDH/DSn Transmitter Output

- 4 Set the **TRANSMIT** display as shown below.

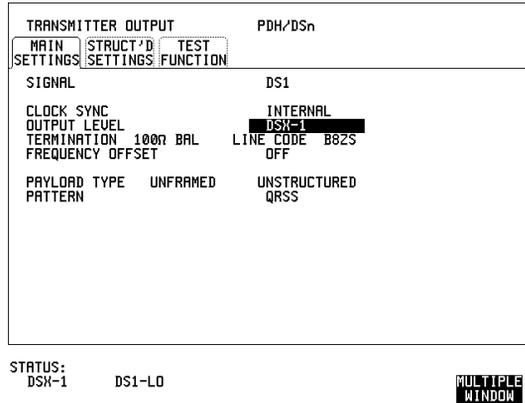

- 5 Select CHAN 1 on the Oscilloscope and set to 1 MΩ input impedance.

Load the Telecom Mask

- 6 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
- SHIFT (Blue Key) APPLICATION.
 - TELECOM MASK/MASK** softkey.
 - Use ENTRY/MEASURE control to select DS1_NEW in the highlighted MSK FILES window.
 - LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 7 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
- RECALL 8, (Ensure CH1 Impedance is reset to 1 MΩ. Select TRIGGER, SETUP and set **PATTERN TRIGGER** softkey to **Trig'd**).
 - DEFINE MEAS
 - COMPARE** softkey
 - TEST ON** softkey
 - M1M2** softkey
 - AFTER FAIL CONTINUE** softkey
 - RUN

Performance Tests

PDH/DSn Transmitter Output

NOTE

Using the balanced to unbalanced converter reduces the pulse amplitude by a factor of 1.266. This will cause the comparison with the mask to fail. To overcome this select CHAN 1 ON and reduce the Volts/Division setting (highlighted on the softkey display). Reduced Volts/Division = highlighted value/1.266. The new value can be entered using the keypad

- 8 The Oscilloscope will compare the positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 9 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 1.896V and 2.844V.

Negative Pulse

- 10 On the Oscilloscope, use the following key sequence to access the inverted mask.
- a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey

Load the Telecom Mask

- 11 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
- a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select DS1_NEW in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 12 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
- a/ RECALL 8, (Ensure CH1 Impedance is reset to 1 M Ω . Select TRIGGER, SETUP and set **PATTERN TRIGGER** softkey to **Trig'd**).
 - b/ DEFINE MEAS

Performance Tests

PDH/DSn Transmitter Output

- c/ **COMPARE** softkey
- d/ **TEST ON** softkey
- e/ **M1M2** softkey
- f/ **AFTER FAIL CONTINUE** softkey
- g/ RUN

NOTE

Using the balanced to unbalanced converter reduces the pulse amplitude by a factor of 1.266. This will cause the comparison with the mask to fail. To overcome this select CHAN 1 ON and reduce the Volts/Division setting (highlighted on the softkey display). Reduced Volts/Division = highlighted value/1.266. The new value can be entered using the keypad

- 13** The Oscilloscope will compare the negative pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 14** Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 1.896V and 2.844V.
- 15** Set the **TRANSMIT** signal to LOW and check that the peak pulse amplitude reduces by approximately 20% and pulse shape has slower rise/fall edges.
- 16** Disconnect all the test equipment.

PDH/DSn Receiver Equalization

Specifications

Rate	Equalization
E1 - 2.048 Mb/s	6 dB for root f cable at 1/2 bit rate
E2 - 8.448 Mb/s	6 dB for root f cable at 1/2 bit rate
E3 - 34.368 Mb/s	12 dB for root f cable at 1/2 bit rate
E4 - 139.264 Mb/s	12 dB for root f cable at 1/2 bit rate
DS1- 1.544 Mb/s	Single range from DS1-LO to DSX -1
DS3 - 44.736 Mb/s	Automatic equalization for up to 900 feet of root f cable.

Description

The Receiver Equalization is checked by looping the transmitter output to receiver input through a special Cable. This simulates the specified cable loss at the rate under test. A BER measurement is run and a check made for no errors in the results page.

Equipment Required

Cable Simulator E4	: 80 metres of 8120-0049
Cable Simulator E3	: 120 metres of 8120-0049
Cable Simulator E2	: 80 metres of 8120-0049
Cable Simulator E1	: 120 metres of 8120-0049
Cable Simulator DS3	: 55 metres of 8120-0049
Cable Simulator DS1	: 80 metres of 8120-0049
110Ω/75Ω Balanced to Unbalanced Converter	: HP 15508B (Qty 2)

Performance Tests


PDH/DSn Receiver Equalization

Procedure

- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4.
- 2 Select **SETTINGS CONTROL** TRANSMITTER and RECEIVER [COUPLED] on the **OTHER** display.

139.264 Mb/s

- 3 Set the **TRANSMIT** display as shown below.

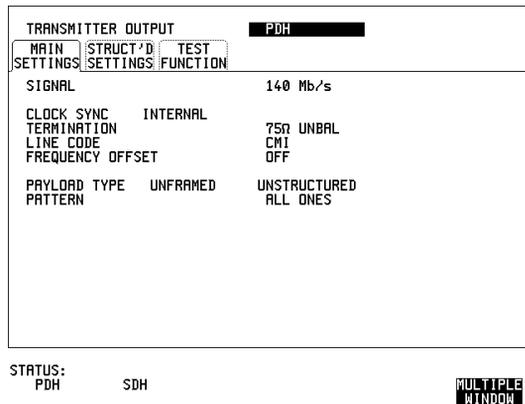


- 4 Connect Cable Simulator E4 between the 139 Mb/s 75Ω OUT and 75Ω IN ports.
- 5 Press **RESULTS** **TROUBLE** **SCAN** then **RUN/STOP** to start the measurement.
- 6 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- 7 Press **RUN/STOP** to stop the measurement.

Performance Tests

PDH/DSn Receiver Equalization

34.368 Mb/s

- 8 Set the **TRANSMIT** display as shown below

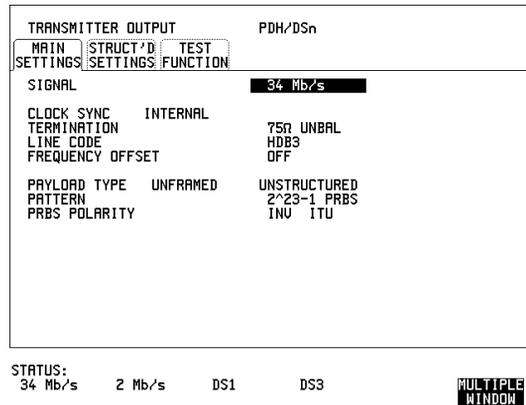


- 9 Connect Cable Simulator E3 between PDH/DSn 75Ω OUT and 75Ω IN ports.
- 10 Press **RESULTS** **TROUBLE** **SCAN** then **RUN/STOP** to start the measurement.
- 11 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- 12 Press **RUN/STOP** to stop the measurement.

Performance Tests

PDH/DSn Receiver Equalization

DS3 (44.736 Mb/s)

13 Set the **TRANSMIT** display as shown below.

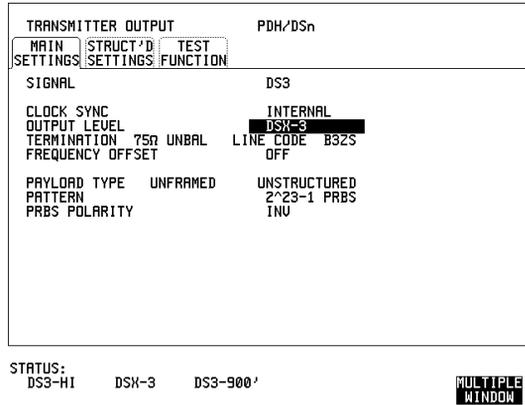

14 Connect Cable Simulator DS3 between the DSn 75Ω OUT and 75Ω IN ports.

15 Press **RESULTS** **TROUBLE** **SCAN** then **RUN/STOP** to start the measurement.

16 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.

17 Press **RUN/STOP** to stop the measurement.

NOTE


If Cable Simulator DS3 is not available, it is permissible to select DS3-900' on the **TRANSMIT** display and connect the HP OmniBER 718 75Ω OUT port direct to the 75Ω IN port. This setup assumes the DS3-900' output signal is within specification.

Performance Tests

PDH/DSn Receiver Equalization

8.448 Mb/s

18 Set the **TRANSMIT** display as shown below.

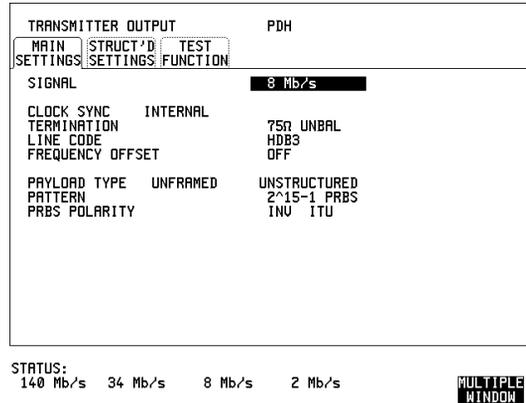

19 Connect Cable Simulator E2 between the PDH/DSn 75Ω OUT and 75Ω IN ports.

20 Press **RESULTS** | **TROUBLE** | **SCAN** then **RUN/STOP** to start the measurement.

21 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.


22 Press **RUN/STOP** to stop the measurement.

Performance Tests

PDH/DSn Receiver Equalization

2.048 Mb/s

23 Set the **TRANSMIT** display as shown below.

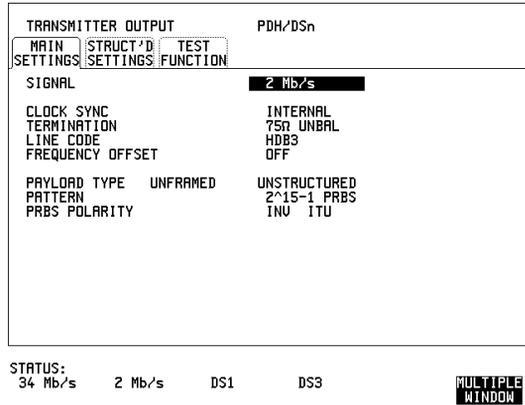

24 Connect Cable Simulator E1 between the PDH/DSn 75Ω OUT and 75Ω IN ports.

25 Press **RESULTS** | **TROUBLE** | **SCAN** then **RUN/STOP** to start the measurement.

26 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.


27 Press **RUN/STOP** to stop the measurement.

Performance Tests

PDH/DSn Receiver Equalization

DS1 (1.544 Mb/s)

28 Set the **TRANSMIT** display as shown below.

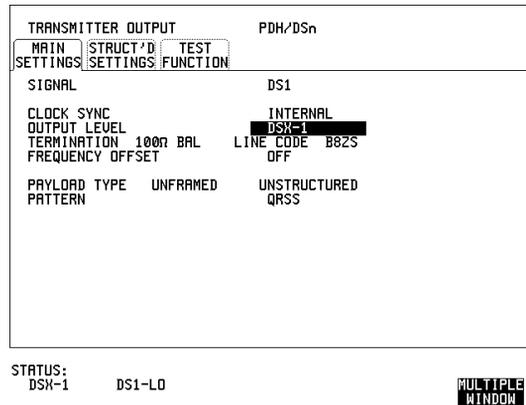

29 Connect Cable Simulator DS1 between the 110Ω OUT and 110Ω IN ports via two Balanced to Unbalanced Converters (HP 15508B).

30 Press **RESULTS** **TROUBLE** **SCAN** then **RUN/STOP** to start the measurement.

31 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.

32 Press **RUN/STOP** to stop the measurement.

NOTE

If Cable Simulator DS1 is not available, it is permissible to select DS1-LO on the **TRANSMIT** display and connect the 110Ω OUT port direct to the 110Ω IN port. This setup assumes the DS1-LO output signal is within specification.

PDH/DSn Receiver Monitor Levels

Specifications

Bit Rate	Nominal Loss	Equalization at 1/2 Bit Rate
E1 - 2.048 Mb/s	20, 26, 30 dB	3 dB
E2 - 8.448 Mb/s	20, 26, 30 dB	3 dB
E3 - 34.368 Mb/s	20, 26 dB	6 dB
E4 - 139.264 Mb/s	20, 26 dB	6 dB
DS1 - 1.544 Mb/s	20, 26, 30 dB	3 dB
DS3 - 44.736 Mb/s	20, 26 dB	6 dB

Description

The signal from the HP OmniBER 718 PDH Transmitter is applied to the PDH Receiver after attenuating by an amount equal to the selected Receiver Flat Loss plus the specified Cable Loss. The Flat Loss is obtained from a 75 Ω attenuator kit. The Cable Loss is supplied by inserting the correct Cable Simulators for each bit rate in the attenuation path.

Equipment Required

Cable Simulator E4-M	: 40 metres of 8120-0049
Cable Simulator E3-M	: 60 metres of 8120-0049
Cable Simulator E2-M	: 40 metres of 8120-0049
Cable Simulator E1-M	: 60 metres of 8120-0049
Cable Simulator DS3	: 55 metres of 8120-0049
Cable Simulator DS1	: 80 metres of 8120-0049
75Ω Attenuator Kit	: HP 86213A
Type N/BNC adaptors	: HP 1250-1534 & -1528 (2 off each)

Performance Tests
PDH/DSn Receiver Monitor Levels

Procedure

- 1 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 2 Connect the equipment as shown in Figure 3-1.


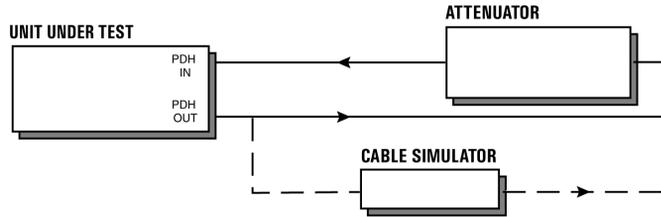


Figure 3-1 Receiver Monitor Input Test Setup

2.048 Mb/s (E1)

- 1 Press **TRANSMIT** and set up the **MAIN SETTINGS** display as shown opposite.

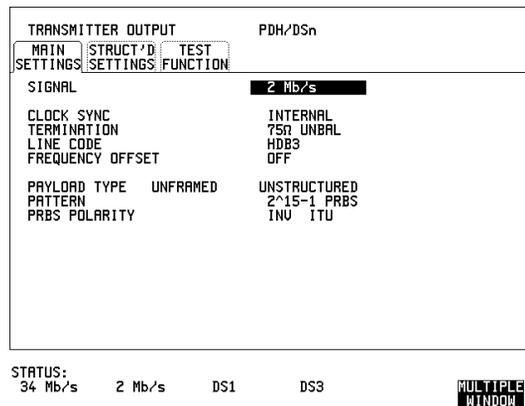

Performance Tests

PDH/DSn Receiver Monitor Levels

- 2 Press **RECEIVE** and set up the **MAIN SETTINGS** display as shown below.

RECEIVER INPUT		PDH/DSn
MAIN SETTINGS	STRUCT'D SETTINGS	TEST FUNCTION
SIGNAL		2 Mb/s
TERMINATION		75Ω UNBAL
LINE CODE		HDB3
LEVEL		MONITOR
EQUALIZER	OFF GAIN	20 dB
PAYLOAD TYPE	UNFRAMED	UNSTRUCTURED
PATTERN		2 ⁿ 15-1 PRBS
PRBS POLARITY		ITU ITU

STATUS:
OFF ON

MULTIPLE WINDOW

- 3 Press **RESULTS TROUBLE SCAN**
- 4 Press **RUN/STOP** to start the measurement.
- 5 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- 6 Press **RUN/STOP** to stop the measurement.
- 7 Press **RECEIVE** and select EQUALIZATION [ON] GAIN [20 dB].
- 8 Connect Cable Simulator E1-M between the PDH OUT Port and the attenuator.
- 9 Press **RESULTS TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 10 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds. Press **RUN/STOP** to stop the measurement.
- 11 Connect the 6 dB Fixed Attenuator in the signal path to give a total path attenuation of 26 dB.
- 12 Press **RECEIVE** and select MONITOR LEVEL [26 dB].
- 13 Press **RESULTS TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 14 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds. Press **RUN/STOP** to stop the measurement.

Performance Tests

PDH/DSn Receiver Monitor Levels

- 15 Remove Cable Simulator E1-M from the signal path.
- 16 Press **RECEIVE** and select EQUALIZATION [OFF].
- 17 Press **RESULTS**; **TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 18 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds. Press **RUN/STOP** to stop the measurement.
- 19 Remove the 6 dB fixed attenuator and connect the 10 dB Fixed Attenuator in the signal path to give a total path attenuation of 30 dB.
- 20 Press **RECEIVE** and set MONITOR LEVEL [30 dB].
- 21 Press **RESULTS**; **TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 22 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds. Press **RUN/STOP** to stop the measurement.
- 23 Press **RECEIVE** and select EQUALIZATION [ON].
- 24 Connect Cable Simulator E1-M between the PDH OUT Port and the attenuator.
- 25 Press **RESULTS**; **TROUBLE SCAN**. Press **RUN/STOP** to start the measurement.
- 26 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds. Press **RUN/STOP** to stop the measurement.

8.448 Mb/s (E2)

- 27 Repeat steps 1 to 26 (20 dB, 26 dB and 30 dB tests) with the HP OmniBER 718 **TRANSMIT** and **RECEIVE** displays set to SIGNAL [8 Mb/s] and Cable Simulator E2-M fitted in place of Cable Simulator E1-M.

34.368 Mb/s (E3)

- 28 Repeat steps 1 to 18 (20 dB and 26 dB tests) with the HP OmniBER 718 **TRANSMIT** and **RECEIVE** displays set to SIGNAL [34 Mb/s] and Cable Simulator E3-M fitted in place of Cable Simulator E1-M.

139.264 Mb/s (E4)

- 29 Repeat steps 1 to 18 (20 dB and 26 dB tests) with the HP OmniBER 718 **TRANSMIT** and **RECEIVE** displays set to SIGNAL [140 Mb/s] and Cable Simulator E4-M fitted in place of Cable Simulator E1-M.

Performance Tests

PDH/DSn Receiver Monitor Levels

1.544 Mb/s (DS-1)

- 30** Repeat steps 1 to 26 (20 dB, 26 dB and 30 dB tests) with the HP OmniBER 718 **TRANSMIT** and **RECEIVE** displays set to SIGNAL [DSX-1]. Connect Cable Simulator DS1 between two Balanced to Unbalanced converters and fit in place of Cable Simulator E1-M.

44.736 Mb/s (DS-3)

- 31** Repeat steps 1 to 18 (20 dB and 26 dB tests) with the HP OmniBER 718 **TRANSMIT** and **RECEIVE** displays set to SIGNAL [DSX-3] and Cable Simulator DS3 fitted in place of Cable Simulator E1-M.
- 32** Disconnect all the test equipment.

External Mux/Demux

Specifications

Rate	Interface	Source
2.048 Mb/s (E1)	Nominally meets ITU-T Rec. G.703 for unbalanced coaxial pair.	Accepts a 2 Mb/s Unbalanced signal conforming to ITU-T Rec. G.703.
1.544 Mb/s (DS-1)	Nominally meets T1.102-1993 for Balanced pair.	Accepts a DS-1 balanced signal conforming to T1.102-1993.

Description

This test verifies operation of the PDH/DSn Mux and demux hardware and confirms the output characteristics of the external demux port on the PDH/DSn Receiver. The *PDH/DSn Test Set* is set up to transmit an unframed 2 Mb/s/DS-1 pattern. This is applied to the HP OmniBER 718 INSERT Port. The 2 Mb/s/DS-1 signal is multiplexed into a 34 Mb/s/DS-3 data stream. The HP OmniBER 718 transmitter and receiver are looped. The unframed 2 Mb/s/DS-1 signal is Demultiplexed from the 34 Mb/s/DS-3 data stream to the *PDH/DSn Test Set via the HP OmniBER 718 DROP* port. A BER test is performed to verify the integrity of the 2 Mb/s/DS-1 signal.

The output from the DROP Port is then applied to an Oscilloscope, and the waveform characteristics are checked to ensure they meet specifications.

Equipment Required

Oscilloscope	: HP 54520A Option 001
PDH Test Set	: HP OmniBER 718
75Ω Termination	: HP 15522-80010
T Connector	: HP 1250-0781

NOTE

The *Test Set* used in this procedure is an HP OmniBER 718. Any other PDH Test Set, capable of generating and measuring at 2 Mb/s/DS-1 unframed, can be used.

Performance Tests
External Mux/Demux

Procedure

2 Mb/s Mux/Demux

- 1 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 2 Connect the equipment as shown in Figure 3-2.


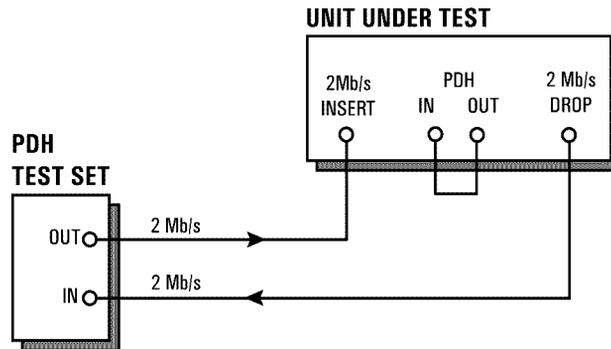


Figure 3-2 External Mux/Demux Test Setup


Performance Tests

External Mux/Demux

- 3 Press **TRANSMIT** on the *Test Set* and set up the display as shown below.

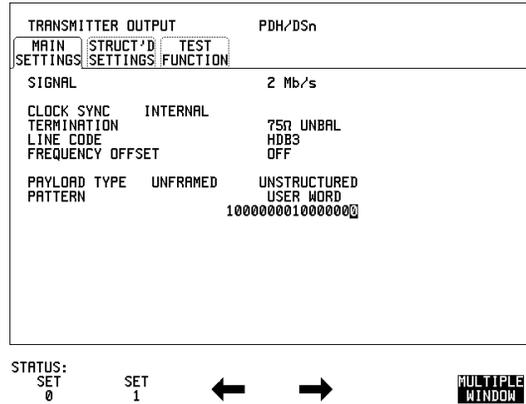


- 4 Press **RECEIVE** on the *Test Set* and set up the display as shown below.

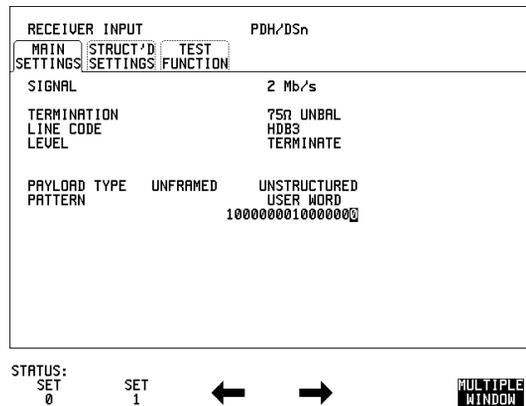

Performance Tests
External Mux/Demux


- 5 Press **TRANSMIT** on the HP OmniBER 718 and set up the **MAIN SETTINGS** display as shown below.

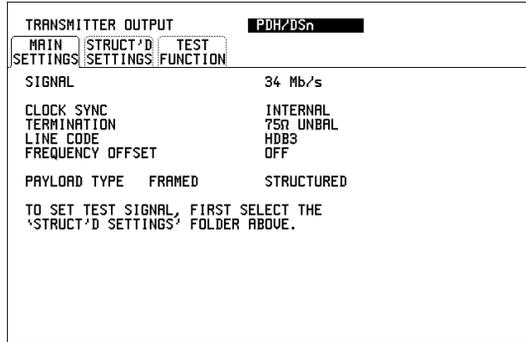

STATUS:

MULTIPLE WINDOW

- 6 Press **TRANSMIT** on the HP OmniBER 718 and set up the **STRUCTURED SETTINGS** display as shown below.

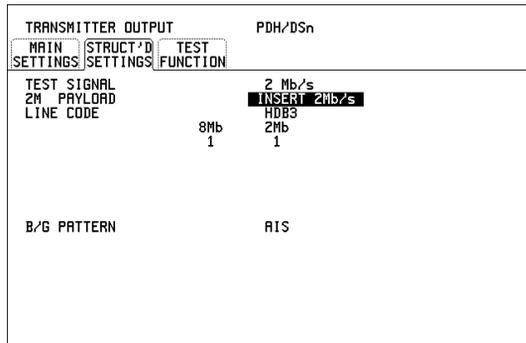

STATUS:

UNFRAMED PCM30 PCM31 PCM30CRC MORE **MULTIPLE WINDOW**

Performance Tests

External Mux/Demux

- 7 Press **RECEIVE** on the HP OmniBER 718 and set up the **MAIN SETTINGS** display as shown below.

RECEIVER INPUT		PDH/DSn
MAIN SETTINGS	STRUCT'D SETTINGS	TEST FUNCTION
SIGNAL		34 Mb/s
TERMINATION		75Ω UNBAL
LINE CODE		HDB3
LEVEL		TERMINATE
PAYLOAD TYPE	FRAMED	STRUCTURED
TO SET TEST SIGNAL, FIRST SELECT THE 'STRUCT'D SETTINGS' FOLDER ABOVE		

STATUS:

MULTIPLE WINDOW

- 8 Press **RECEIVE** on the HP OmniBER 718 and set up the **STRUCTURED SETTINGS** display as shown below.

RECEIVER INPUT		PDH/DSn
MAIN SETTINGS	STRUCT'D SETTINGS	TEST FUNCTION
TEST SIGNAL		2 Mb/s
2M PAYLOAD		DRDF 2Mb/s
LINE CODE		HDB3
	8Mb	2Mb
	1	1

STATUS:

UNFRAMED

PCM30

PCM31

PCM30CRC

MORE

MULTIPLE WINDOW

- 9 Press **RUN/STOP** on the Test Set. Press **RESULTS TROUBLE SCAN** on the Test Set and ensure that NO TROUBLE is displayed.
- 10 Press SINGLE error add key on the Test Set and ensure the Bit Error count increments by one each time the key is pressed.

Performance Tests

External Mux/Demux

2.048 Mb/s Positive Pulse

- 11 Disconnect the UUT 75 Ω DROP port from the Test Set and connect to the Oscilloscope. Terminate in 75 Ω at the Oscilloscope input.
- 12 Select CHAN 1 on the Oscilloscope and set to 1 M Ω input impedance.

Load the Telecom Mask

- 13 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select DS_1E in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 14 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 15 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 16 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 2.37 Volts.

2.048 Mb/s Negative Pulse

- 17 On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey

Performance Tests

External Mux/Demux

- c/ Use ENTRY/MEASURE control to highlight INV_MASK
- d/ **CHANGE DIRECTORY** softkey

Load the Telecom Mask

- 18** On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
- a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select DS_1E in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 19** On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
- a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 20** The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 21** Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is approximately 2.37 Volts.

DS-1 Mux and Demux

- 1** Connect the UUT balanced DS-1 Insert and Drop ports to the DS-1 Balanced Ports of the Test Set and repeat steps 3 through 10 substituting DS-1 for 2 Mb/s and DS-3 for 34 Mb/s.

Performance Tests

External Mux/Demux

DS-1 Positive Pulse

- 2 Disconnect the UUT 100 Ω DROP port from the Test Set and connect to the Oscilloscope via the HP 15508B Balanced to unbalanced Converter. Terminate in 75 Ω at the Oscilloscope input.
- 3 Select CHAN 1 on the Oscilloscope and set to 1 M Ω input impedance.

Load the Telecom Mask

- 4 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select DS1_NEW in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 5 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8, (Ensure CH1 Impedance is reset to 1 M Ω . Select TRIGGER, SETUP and set **PATTERN TRIGGER** softkey to **Trig'd**).
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN

NOTE

Using the balanced to unbalanced converter reduces the pulse amplitude by a factor of 1.266. This will cause the comparison with the mask to fail. To overcome this select CHAN 1 ON and reduce the Volts/Division setting (highlighted on the softkey display). Reduced Volts/Division = highlighted value/1.266. The new value can be entered using the keypad

- 6 The Oscilloscope will compare the positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

Performance Tests

External Mux/Demux

- 7 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 1.896V and 2.844V.

DS-1 Negative Pulse

- 8 On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey

Load the Telecom Mask

- 9 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select DS1_NEW in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 10 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8, (Ensure CH1 Impedance is reset to 1 M Ω . Select TRIGGER, SETUP and set **PATTERN TRIGGER** softkey to **Trig'd**).
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN

NOTE

Using the balanced to unbalanced converter reduces the pulse amplitude by a factor of 1.266. This will cause the comparison with the mask to fail. To overcome this select CHAN 1 ON and reduce the Volts/Division setting (highlighted on the softkey display). Reduced Volts/Division = highlighted value/1.266. The new value can be entered using the keypad

- 11 The Oscilloscope will compare the negative pulse with the mask limits. A PASS message should appear on the Oscilloscope.

Performance Tests
External Mux/Demux

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 12** Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 1.896V and 2.844V.
- 13** Disconnect all test equipment.

PDH/DSn Frequency Measurement and Looped Clock

Specifications

Accuracy	±4.5 ppm
Measured Offset	±100 ppm

Description

This test verifies that the HP OmniBER 718 Receiver Frequency Measurement is within specified limits. These limits assume the instrument is within the calibration cycle.

A Synthesizer is used to generate a sinewave at half the data rate. This is applied to the HP OmniBER 718 Receiver Signal In port. As this signal corresponds to an *All Ones Ternary Signal*, the HP OmniBER 718 receiver should sync up with no errors if set to PATTERN [ALL ONES]. The Frequency Measurement accuracy of the HP OmniBER 718 can be determined by comparison with the frequency displayed on the Synthesizer. Frequency Offset Measurement is also verified during this test as the HP OmniBER 718 will display deviation from the expected Signal In frequency in ppm. The PDH transmitter recovered clock function is also verified at 2 Mb/s using the frequency counter in RATIO mode.

Equipment Required

Synthesizer : HP 3335A Option 001 (75Ω)
Frequency Counter : HP 5335A Option 010

Procedure

- 1 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 2 Connect up the equipment as shown in Figure 3-3.

Performance Tests
PDH/DSn Frequency Measurement and Looped Clock


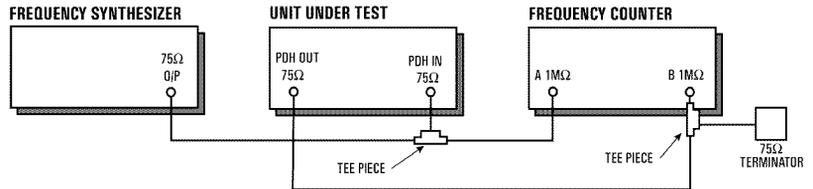


Figure 3-3 Receiver Frequency Measurement Test Setup


- 3 Set the Synthesizer to:
 FREQUENCY - 1024.000 kHz sinewave
 AMPLITUDE - +10 dBm.
- 4 Set the frequency counter to RATIO A/B.
- 5 Press **RECEIVE** and set up the display as shown below.

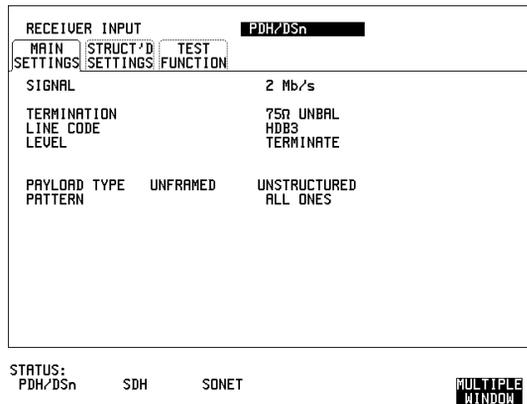


Performance Tests

PDH/DSn Frequency Measurement and Looped Clock

- 6 Press **TRANSMIT** and set up the display as shown below.

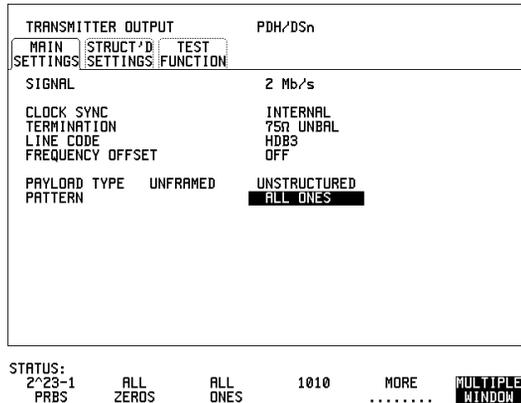

- 7 Press **RESULTS** and set up the display as shown below.

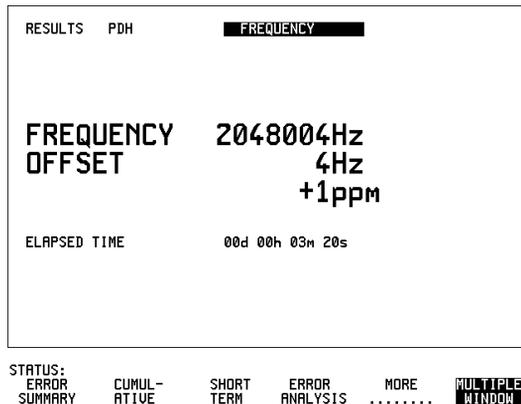

- 8 Verify that the FREQUENCY displayed is between 2047991 Hz and 2048009 Hz.
- 9 Verify that the Offset displayed is between +4.5 ppm and -4.5 ppm.
- 10 Set the synthesizer frequency to 1024.102 kHz and verify that the frequency displayed on the **RESULTS** display is between 2048.194 kHz and 2048.214 kHz.

Performance Tests

PDH/DSn Frequency Measurement and Looped Clock

- 11 Verify that the Offset displayed is between 95.5 ppm and 104.5 ppm. The frequency counter should read 1.00.
- 12 Set the synthesizer frequency to 1023.898 kHz and verify that the frequency displayed on the **RESULTS** display is between 2047.786 kHz and 2047.806 kHz.
- 13 Verify that the Offset displayed is between -95.5 ppm and -104.5 ppm. The frequency counter should read 1.00.
- 14 Set the synthesizer level to +10 dBm, synthesizer frequency and the Omniber 718 to the settings given in Table 3-2 and verify the displayed Offset at each point.

Table 3-2 PDH/DSn Offsets

Receive Frequency	Synthesizer Frequency	Displayed Offset
8 Mb/s (E2)	4224,000 Hz	-4.5 to +4.5 ppm
8 Mb/s (E2)	4223,578 Hz	-95.5 to -104.5 ppm
8 Mb/s (E2)	4224,422 Hz	+95.5 to +104.5 ppm
34 Mb/s (E3)	17,184,000 Hz	-4.5 to +4.5 ppm
34 Mb/s (E3)	17,182,282 Hz	-95.5 to -104.5 ppm
34 Mb/s (E3)	17,185,718 Hz	+95.5 to +104.5 ppm
140 Mb/s (E4)	69,632,000 Hz	-4.5 to +4.5 ppm
140 Mb/s (E4)	69,625,036 Hz	-95.5 to -104.5 ppm
140 Mb/s (E4)	69,638,963 Hz	+95.5 to +104.5 ppm
1.544 Mb/s (DS-1)	772,000 Hz	-4.5 to +4.5 ppm
1.544 Mb/s (DS-1)	771,923 Hz	-95.5 to -104.5 ppm
1.544 Mb/s (DS-1)	772,077 Hz	+95.5 to +104.5 ppm
44.736 Mb/s (DS-3)	22,368,000 Hz	-4.5 to +4.5 ppm
44.736 Mb/s (DS-3)	22,365,763 Hz	-95.5 to -104.5 ppm
44.736 Mb/s (DS-3)	22,370,237 Hz	+95.5 to +104.5 ppm

SDH/SONET Transmitter Clock Accuracy

Specification

Bit Rate	Accuracy
51.84 Mb/s	±4.5 ppm

Description

The test uses a Frequency Counter connected to the Multirate Analyzer module Clock Trigger output port. This output is derived from the Clock module internal 10 MHz clock oscillator providing a 51.84 MHz that is directly related to all SDH/SONET output rates.

Equipment Required

Frequency Counter : HP 5335A Option 010

Procedure

- 1** Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 2** Set the Transmitter Output to SDH/SONET.
- 3** Connect the HP OmniBER 718 Multirate Analyzer module CLOCK TRIGGER port to the Frequency Counter Input A, set the input termination to 50 Ω .
- 4** Adjust the Frequency Counter Trigger Level to obtain a stable reading and ensure that the Frequency Counter reads between 51.839670 MHz and 51.840230 MHz.
- 5** Disconnect all the test equipment.

External Clock/Data Reference Inputs & Clock Reference Output

Specifications

Clock Rate	Description
2.048 Mb/s MTS	Accepts timing reference as per ITU-T G.811
10 MHz Reference	Accepts 10 MHz timing reference
1.544 Mb/s BITS	Accepts DS-1 timing reference as per TA-TSY-000378
64 kb/s	Accepts 64 kb/s timing reference as per ITU-T G.703 Section 1.2.2
STM-1/STS-3 Receive	Recovers clock from received STM/STS input signal.

NOTE

The rates available are dependent on the HP OmniBER 718 model and options fitted.

Description

This test verifies that signal integrity is maintained when an EXTERNAL clock is used as a reference.

Equipment Required

Synthesizer : HP 3335A option 001 (75 Ω)

PDH/DSn Test Set : HP OmniBER 718

110 Ω /75 Ω Balanced to Unbalanced Converter : HP 15508B

Frequency Counter : HP 5335A Opt 010

64kb/s Test Set : HP 37732A


Performance Tests

External Clock/Data Reference Inputs & Clock Reference Output


Procedure

MTS Clock - Clock Format

- 1 Connect the 52/155 Mb/s DATA OUT port to the 52/155 Mb/s DATA IN port.
- 2 Recall the HP OmniBER 718 Default Settings as shown on page 3-4 and set the **OTHER** **SETTINGS** **CONTROL** display as shown below.

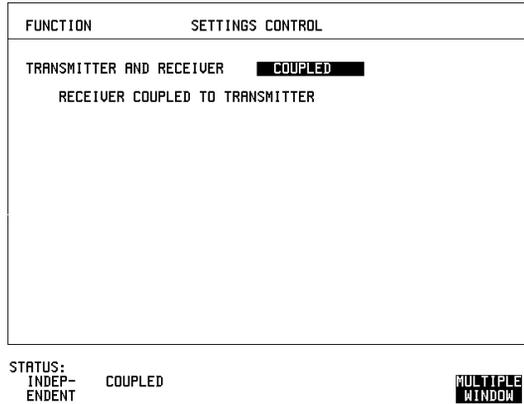

- 3 Press **TRANSMIT** and set up the display as shown below.

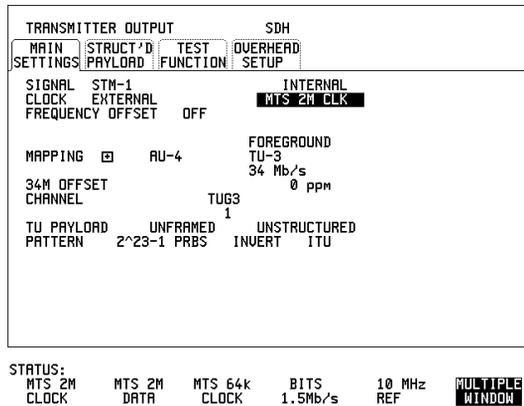

- 4 Set the HP 3335A to 2.048 MHz at +10 dBm.

Performance Tests

External Clock/Data Reference Inputs & Clock Reference Output


- 5 Connect the HP 3335A to the HP OmniBER 718 75Ω 2M REF IN port on the Clock module.
- 6 Press **RESULTS**; **TROUBLE SCAN**.
- 7 Press **RUN/STOP**, check that the display reads NO TROUBLE and all the Alarm leds are off.
- 8 Press **RUN/STOP** to halt the measurement.

Clock REF OUT

- 9 Connect the Clock REF Out port to the Frequency Counter and check that a 2.048 MHz signal is present.

MTS Clock - Data

- 10 Disconnect the HP 3335A Synthesizer from the HP OmniBER 718 75Ω 2M REF IN port.
- 11 Set the PDH/DSn Test Set to transmit a 2 Mb/s unframed signal.
- 12 Connect the PDH/DSn Test Set, 75Ω Output to the HP OmniBER 718 75Ω 2M REF IN Port and Recall the DEFAULT SETTINGS as shown on page 3-4.
- 13 Set the **TRANSMIT** display as shown below.

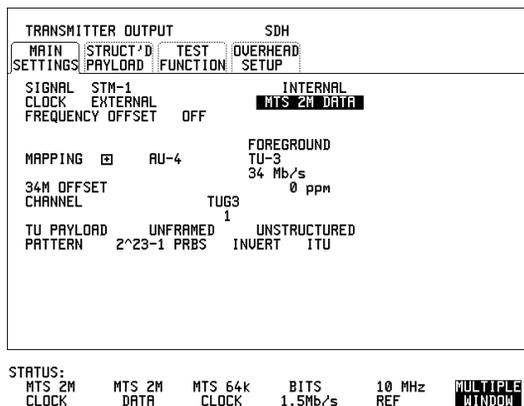

- 14 Select CLOCK SYNC FORMAT [2 Mb/s DATA] on the SDH **TRANSMIT** Display.
- 15 Press **RESULTS** **TROUBLE SCAN** then **RUN/STOP**.

Performance Tests

External Clock/Data Reference Inputs & Clock Reference Output

- 16 Check that the **RESULTS** Display reads NO TROUBLE and all the Alarm LEDs are off. Press **RUN/STOP** to halt the measurement.
- 17 Disconnect the PDH/DSn Test Set, 75 Ω 2 Mb/s PDH Output from the 75 Ω 2M REF IN Port.
- 18 Connect the PDH/DSn Test Set, 120 Ω 2 Mb/s PDH Output to the 120 Ω 2M REF IN Port.
- 19 Change the PDH O/P termination to 120 Ω on the PDH/DSn Test Set and the HP OmniBER 718.
- 20 Press **RESULTS** **TROUBLE SCAN** then **RUN/STOP** on the HP OmniBER 718.
- 21 Check that the **RESULTS** Display reads NO TROUBLE and all the Alarm LEDs are off. Press **RUN/STOP** to halt the measurement.

STM-1/STS-3 Receive Data

- 22 Disconnect the PDH/DSn Test Set Data Output from the HP OmniBER 718, 120 Ω 2M REF IN port.
- 23 Disconnect the 52/155 Mb/s DATA OUT port from the 52/155 Mb/s DATA IN port
- 24 Select CLOCK SYNC [STM-1/STS-3 RECEIVE] ON THE HP OmniBER 718 **TRANSMIT** display.
- 25 The SDH Clock Loss Alarm led should be lit on the HP OmniBER 718.
- 26 Set the Synthesizer frequency to 77.760 MHz and amplitude to +10 dBm.
- 27 Connect the Synthesizer to the 75 Ω 52/155 Mb/s DATA IN port.
- 28 Ensure that the SDH/SONET Clock Loss Alarm Led is not lit.

NOTE

As the signal is unframed the LOF/OOF etc. alarms will be on.

10 MHz Reference

- 29 Select CLOCK SYNC [10 MHz REF] ON THE HP OmniBER 718 **TRANSMIT** display.
- 30 The SDH/SONET Clock Loss Alarm led should be lit on the HP OmniBER 718.
- 31 Set the Synthesizer frequency to 10.000 MHz and amplitude to +10 dBm.

Performance Tests

External Clock/Data Reference Inputs & Clock Reference Output

32 Connect the Synthesizer to the HP OmniBER 718, 75 Ω 2M REF IN Port.

33 Ensure that the SDH/SONET Clock Loss Alarm Led is not lit.

BITS Clock

34 Select CLOCK SYNC [BITS] ON THE HP OmniBER 718 **TRANSMIT** display.

35 The SDH/SONET Clock Loss Alarm led should be lit on the HP OmniBER 718.

36 Set the Synthesizer frequency to 772 kHz and amplitude to +10 dBm.

37 Connect the Synthesizer, via the Balanced to Unbalanced converter, to the HP OmniBER 718, 100 Ω BITS Clock Port.


38 Ensure that the SDH/SONET Clock Loss Alarm Led is not lit.

64 kb/s Clock

39 Select CLOCK SYNC [64 kb/s] on the HP OmniBER 718 **TRANSMIT** display.

40 The SDH/SONET Clock Loss Alarm led should be lit on the HP OmniBER 718.

41 Set the 64kb/s Test Set to provide a 64kb/s Clock Signal.

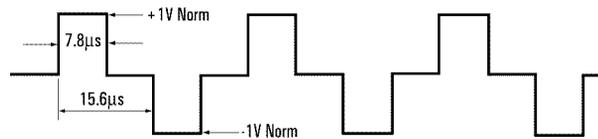

Suitable 64kb/s AMI signal (into 100/120 ohms balanced)
if 64kb/s Test set is not available.
Signal must be derived from a stable synthesized source.

42 Connect the Clock Signal to the HP OmniBER 718 balanced 64K Clock input.

43 Ensure that the SDH/SONET Clock Loss Alarm Led is not lit.

44 Disconnect all the test equipment.

SDH/SONET Frequency Offsets

Specifications

Range	±999 ppm
Resolution	0.1 ppm
Accuracy	0.02 ppm

Description

The test uses a Frequency Counter connected to the Multirate Analyzer module Clock Trigger output port. This output is derived from the Clock module and is directly related to the SDH/SONET output rate. An external 10 MHz reference from a Signal Generator is used to clock the HP OmniBER 718 and also provides a timebase reference for the Frequency counter. The counter measures the Clock Trigger frequency to check the offset accuracy and range.

Equipment Required

Signal Generator	: HP 8657A
Frequency Counter	: HP 5335A Opt 010
T Connector	: HP 1250-0781

Procedure

- 1 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4. Set the Transmitter Output to SDH/SONET.
- 2 Select CLOCK SYNC [10 MHz REF] on the HP OmniBER 718 **TRANSMIT** display.
- 3 Connect the HP8657A to the HP OmniBER 718 Unbalanced 75Ω 2M REF IN port on the Clock Module.
- 4 Set the Signal Generator frequency to 10.000 MHz and amplitude to +10 dBm.
- 5 Check the Clock Loss Alarm Led is not lit.

Performance Tests

SDH/SONET Frequency Offsets

- 6 Connect the Signal Generator, Timebase OUT port (rear panel), to the counter Timebase IN port (rear panel).
- 7 Check the Counter EXT TIME BASE flag is illuminated on the front panel.
- 8 Connect the HP OmniBER 718 Multirate Analyzer module CLOCK TRIGGER port to the Frequency Counter, set input termination to 50Ω .
- 9 Adjust the Frequency Counter Trigger Level to obtain a stable reading.
- 10 The reading should be between 51.839999 - 51.840001 MHz. If not check setup and ensure the Counter is locked to the Signal Generator.
- 11 Set the HP OmniBER 718 frequency offset to the settings given in Table 3-3 and verify the frequency at each step is within the Min/Max limits.

Table 3-3 SDH/SONET Offset

Offset (ppm)	Min Expected Frequency	Max Expected Frequency
-999ppm	51788210.8 Hz	51788212.9 Hz
-100ppm	51834814.9 Hz	51834817.1 Hz
-66.6ppm	51836546.4 Hz	51836548.5 Hz
+33.3ppm	51841725.2 Hz	51841727.3 Hz
+100ppm	51845182.9 Hz	51845185.1 Hz
+999ppm	51891787.1 Hz	51891789.2 Hz

- 12 Disconnect all the test equipment.

STM-0/STS-1 Transmitter Output Waveshape

Specifications

Level	Pulse Amplitude & Shape
Cross-Connect (450 feet)	530 mV peak (nominal). Compliant with GR-253, Issue 1, Figure 4-10 and draft recommendation ITU-R F.750, Appendix1
HIGH	1 V peak (nominal)
LOW	300 mV peak (nominal)

Description

An Oscilloscope is connected to the HP OmniBER 718 Transmitter STM-0/STS-1 output and used to check the STM-0/STS-1 waveshape against the relevant mask.

Equipment Required

Oscilloscope : HP 54520A Option 001
75 Ω Termination : HP 15522-80010
T Connector : HP 1250-0781

Procedure

Positive Pulse

- 1 Recall HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4 and set up the **TRANSMIT** display as shown on the following page.

Performance Tests

STM-0/STS-1 Transmitter Output Waveshape

TRANSMITTER OUTPUT		SDH	
MAIN SETTINGS	STRUCT'D PAYLOAD	TEST FUNCTION	OVERHEAD SETUP
SIGNAL	STM-0	X-CON	INTERNAL
CLOCK	INTERNAL		
FREQUENCY OFFSET	OFF		
MAPPING	<input checked="" type="checkbox"/> AU-3	FOREGROUND	UC-3
34M OFFSET		34 Mb/s	0 ppm
PAYLOAD TYPE	UNFRAMED	UNSTRUCTURED	
PATTERN	2^23-1 PRBS	INVERT	ITU

STATUS: CROSS-CONNECT HIGH LOW **MULTIPLE WINDOW**

- 2 Connect the 52/155 Mb/s 75Ω DATA OUT port to the Oscilloscope CHAN 1, terminate in 75Ω.
- 3 Select CHAN 1 on the Oscilloscope and set to 1 MΩ input impedance.

Load the Telecom Mask

- 4 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select STS1_93 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 5 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 6 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

STM-0/STS-1 Transmitter Output Waveshape

NOTE

It may be necessary to select **MASK** softkey and **MASK AUTO** / **MASK ALIGN** or to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical gain/ position and horizontal delay to obtain a PASS on the Mask.

- 7 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is nominally 530 mV.

Negative Pulse

- 8 On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey

Load the Telecom Mask

- 9 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select STS1_93 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 10 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 11 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

Performance Tests

STM-0/STS-1 Transmitter Output Waveshape

NOTE

It may be necessary to select **MASK** and **MASK AUTO** / **MASK ALIGN** to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical gain/position and horizontal delay to obtain a PASS on the Mask.

- 12** Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is nominally 530 mV.
- 13** Change the signal to STM-0/STS-1 HIGH and check that the +ve and -ve pulses are nominally 1 V.
- 14** Change the signal to STM-0/STS-1 LOW and check that the +ve and -ve pulses (max) peaks are nominally 300 mV.

STM-1/STS-3 Transmitter Output Waveshape

Specifications

Pulse Shape	Meets ITU Recommendation G.703
Amplitude	$\pm 0.5V \pm 10\%$

Description

An Oscilloscope is connected to the HP OmniBER 718 Transmitter STM-1/STS-3 output and used to view the waveforms with All Ones and All Zeros patterns selected in turn. The displayed waveshape is checked against the relevant mask. The STM/STS Framing is disabled during this test.

Equipment Required

Oscilloscope	HP 54520A - option 001
75Ω Termination	HP 15522-80010
T Connector	HP 1250-0781

Procedure

NOTE

This performance test is written using the HP 54520A Oscilloscope with Option 001 - Telecom Masks Application. If any other Oscilloscope is used the keystrokes given in this procedure will not apply.

Installing the Telecom Masks Option

- 1 Insert the Disk containing the Telecom Mask into the Oscilloscope Disk Drive.
- 2 Press **SHIFT** (Blue Key) **DISK**
- 3 Press **DIRECTORY** then **ROOT DIRECTORY**.

Performance Tests

STM-1/STS-3 Transmitter Output Waveshape

All Ones Pulse

- 1 Connect up the equipment as shown in Figure 3-4 and Recall HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.


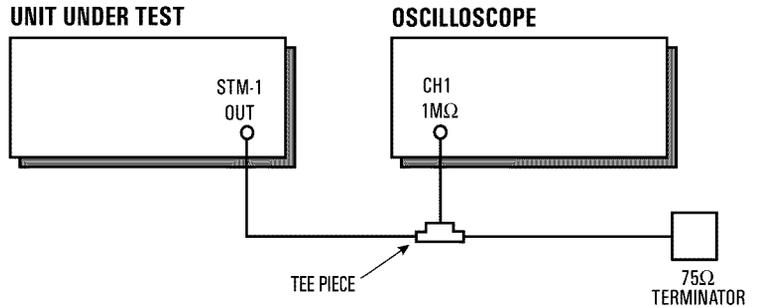


Figure 3-4

STM-1/STS-3 Transmitter Output Waveshape Test Setup


- 2 Press **TRANSMIT** and set up the display as shown below.

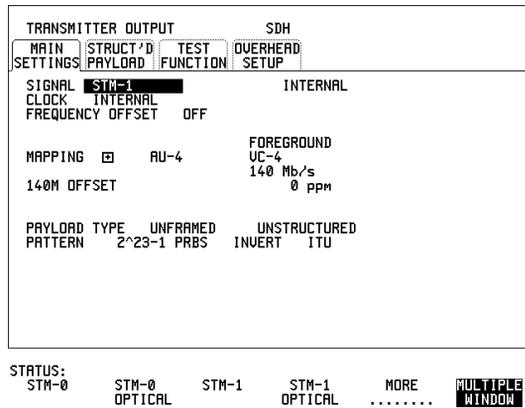

Performance Tests

STM-1/STS-3 Transmitter Output Waveshape

- 3 Press **OTHER** **CALIBRATION** and enter the calibration password - 1243. Set up the display as shown opposite.

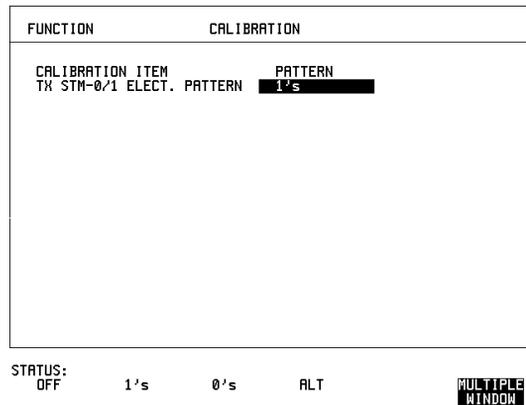

- 4 Connect the 52/155 Mb/s 75Ω DATA OUT port to the Oscilloscope, terminate in 75Ω.
- 5 Select CHAN on the Oscilloscope and set to 1 MΩ input impedance.

Load the Telecom Mask

- 6 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
 - a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 155BIN1 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 7 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
 - a/ RECALL 8, (Ensure CH1 Impedance is reset to 1 MΩ)
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN

Performance Tests

STM-1/STS-3 Transmitter Output Waveshape

- 8 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 9 Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 450 mV and 550 mV. (i.e. 900 mV-1.1V Pk-Pk)

All 0's Pulse

- 10 Select PATTERN [ALL 0's] on the **OTHER** **CALIBRATION** display.

Load the Telecom Mask

- 11 On the Oscilloscope, use the following key sequence to select and load the required Telecom Mask:
- a/ SHIFT (Blue Key) APPLICATION.
 - b/ **TELECOM MASK/MASK** softkey.
 - c/ Use ENTRY/MEASURE control to select 155BIN0 in the highlighted MSK FILES window.
 - d/ **LOAD SETUP 8 M1M2** softkey.

Compare Pulse with Mask

- 12 On the Oscilloscope, use the following key sequence to compare the pulse with the mask:
- a/ RECALL 8, (Ensure CH1 Impedance is reset to 1 M Ω)
 - b/ DEFINE MEAS
 - c/ **COMPARE** softkey
 - d/ **TEST ON** softkey
 - e/ **M1M2** softkey
 - f/ **AFTER FAIL CONTINUE** softkey
 - g/ RUN
- 13 The Oscilloscope will automatically display and compare an isolated positive pulse with the mask limits. A PASS message should appear on the Oscilloscope.

Performance Tests

STM-1/STS-3 Transmitter Output Waveshape

NOTE

It may be necessary to visibly fit the waveform to the mask by adjusting the Oscilloscope vertical position and horizontal delay to obtain a PASS on the Mask.

- 14** Measure the peak pulse amplitude at the mid pulse-width using the Oscilloscope and verify that this is between 450 mV and 550 mV. (i.e. 900 mV-1.1V Pk-Pk)
- 15** On the Oscilloscope, use the following key sequence to access the inverted mask.
 - a/ SHIFT (Blue Key) DISK
 - b/ **DIRECTORY** softkey
 - c/ Use ENTRY/MEASURE control to highlight INV_MASK
 - d/ **CHANGE DIRECTORY** softkey
- 16** Repeat steps 6 to 14 to check pulses against Inverted masks.
- 17** Set CALIBRATION PATTERN to OFF and disconnect all the test equipment.

SDH/SONET Receiver Equalization

Specifications

Rate	Equalization
STM-0/STS-1 - 51.84 Mb/s	12 dB for root f cable at 1/2 bit rate
STM-1/STS-3 - 155.52 Mb/s	12 dB for root f cable at 1/2 bit rate

Description

The Receiver Equalization is checked by looping the transmitter output to receiver input through a special Cable Simulator. This device is designed to simulate the specified cable loss at the rate under test. A BER measurement is run and a check made for no errors in the results page.

Equipment Required

Cable Simulator STM-0/STS-1 50 metres of 8120-0049

Cable Simulator STM-1/STS-3 75 metres of 8120-0049


Procedure

STM-0/STS-1


- 1 Recall the HP OmniBER 718 Default Settings as shown on page 3-4 and set the **OTHER** **SETTINGS** **CONTROL** display as shown on the following page.

Performance Tests

SDH/SONET Receiver Equalization

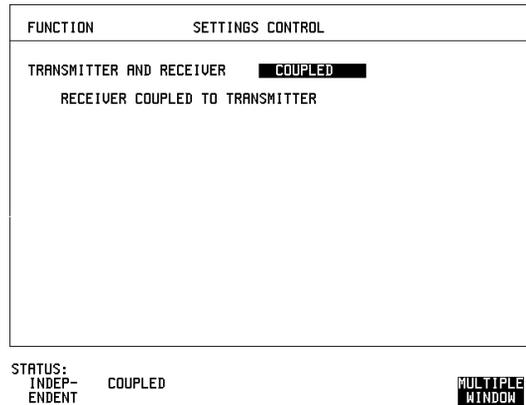

- Set the **TRANSMIT** display as shown below.

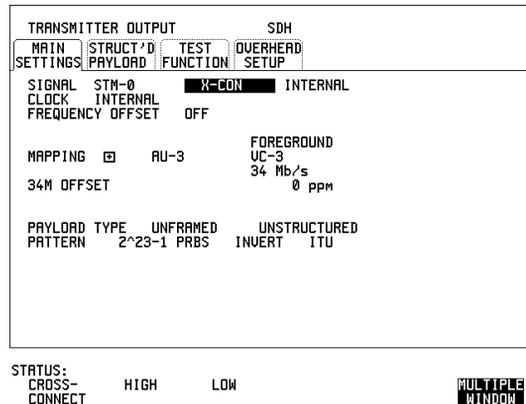

- Connect Cable Simulator STS-1 between the 52/155 Mb/s 75Ω DATA OUT and 52/155 Mb/s 75Ω DATA IN ports.
- Press **RESULTS** **TROUBLE** **SCAN** then **RUN/STOP** to start the measurement.
- Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- Press **RUN/STOP** to stop the measurement.

Performance Tests

SDH/SONET Receiver Equalization

Procedure

STM-1/STS-3

Set the **TRANSMIT** display as shown below.

7

TRANSMITTER OUTPUT		SDH	
MAIN	STRUCT'D	TEST	OVERHEAD
SETTINGS	PAYLOAD	FUNCTION	SETUP
SIGNAL	STM-1		INTERNAL
CLOCK	INTERNAL		
FREQUENCY OFFSET	OFF		
MAPPING	<input checked="" type="checkbox"/> AU-4		BACKGROUND
140M OFFSET			UC-4
			140 Mb/s
			0 ppm
PAYLOAD TYPE	UNFRAMED		UNSTRUCTURED
PATTERN	2^23-1 PRBS	INVERT	ITU

STATUS:
STM-0 STM-0 STM-1 STM-1 MORE MULTIPLE
 OPTICAL OPTICAL

- 8 Connect Cable Simulator STS-3 between the 52/155 Mb/s 75Ω DATA OUT and 52/155 Mb/s 75Ω DATA IN ports.
- 9 Press **RESULTS** **TROUBLE** **SCAN** then **RUN/STOP** to start the measurement.
- 10 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- 11 Press **RUN/STOP** to stop the measurement.
- 12 Disconnect all the equipment.

SDH/SONET Receiver Monitor Levels

Specifications

Bit Rate	Nominal Loss	Equalization at 1/2 Bit Rate
STM-0/STS-1 - 51.84 Mb/s	20, 26 dB	12 dB
STM-1/STS-3 - 155.52 Mb/s	20, 26 dB	12 dB

Description

The signal from the HP OmniBER 718 SDH/SONET Transmitter is applied to the SDH/SONET Receiver after attenuating by an amount equal to the selected Receiver Flat Loss plus the specified Cable Loss. The Flat Loss is obtained from a 75 Ω attenuator kit. The Cable Loss is supplied by inserting the correct Cable Simulators for each bit rate in the attenuation path.

Equipment Required

Cable Simulator STM-0/STS-1 50 metres of 8120-0049

Cable Simulator STM-1/STS-3 75 metres of 8120-0049

75 Ω Attenuator Kit HP 86213A

Procedure

- 1 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 2 Connect the equipment as shown in Figure 3-5.

Performance Tests
SDH/SONET Receiver Monitor Levels


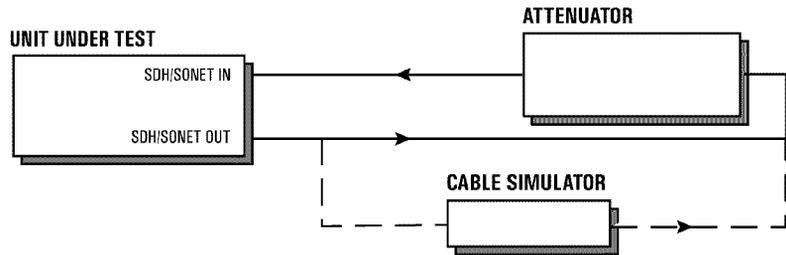


Figure 3-5 Receiver Monitor Input Test Setup

STM-0/STS-1

- 1 Set the **OTHER** **SETTINGS** **CONTROL** display as shown below.

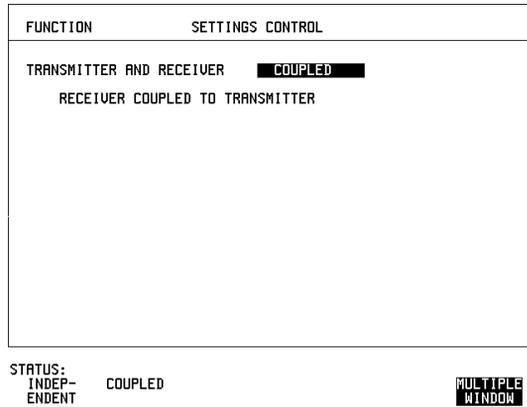

Performance Tests

SDH/SONET Receiver Monitor Levels

- 2 Press **RECEIVE** and set up the **MAIN SETTINGS** display below.

RECEIVER INPUT		SDH	
MAIN SETTINGS	STRUCT'D PAYLOAD	TEST FUNCTION	OVERHEAD MONITOR
SIGNAL LEVEL		STM-0 MONITOR	
GAIN		20 dB	
MAPPING	RU-3	UC-3	34 Mb/s
PAYLOAD TYPE	UNFRAMED	UNSTRUCTURED	
PATTERN	2 ²³ -1 PRBS	INVERT	ITU

STATUS:
20 dB 26 dB **MULTIPLE WINDOW**

- 3 Press **RESULTS TROUBLE SCAN**
- 4 Press **RUN/STOP** to start the measurement.
- 5 After 30 seconds ensure that NO TROUBLE is displayed on the **RESULTS** display
- 6 Press **RUN/STOP** to stop the measurement.
- 7 Connect Cable Simulator STS-1 between the 52/155 Mb/s DATA OUT Port and the attenuator.
- 8 Press **RESULTS TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 9 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- 10 Press **RUN/STOP** to stop the measurement.
- 11 Connect the 6 dB Fixed Attenuator in the signal path to give a total path attenuation of 26 dB.
- 12 Press **RECEIVE** and select MONITOR LEVEL [26 dB].
- 13 Press **RESULTS TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 14 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- 15 Press **RUN/STOP** to stop the measurement.
- 16 Remove Cable Simulator STS-1 from the signal path.

Performance Tests

SDH/SONET Receiver Monitor Levels

- 17 Press **RESULTS**; **TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 18 Ensure that NO TROUBLE is displayed on the **RESULTS** display after 30 seconds.
- 19 Press **RUN/STOP** to stop the measurement.

STM-1/STS-3

- 20 Repeat steps 1 to 19 (20 dB and 26 dB tests) with the **RECEIVE** display set to SIGNAL [STM-1/STS-3] and Cable Simulator STS-3 fitted in place of Cable Simulator STS-1.
- 21 Disconnect all the equipment.

Multirate Optical Interfaces

Specification (1310 nm Transmitter up to 622 Mb/s)

Wavelength	1280 nm to 1335 nm (Typical 1310 nm)
Power Output	-3.0 dBm to +2.0 dBm (Typical 0.0 dBm)
Line Coding	NRZ
Safety Class	Class 1, FDA 21 CFR Ch.1 1040.10 and EN 60825
Data Rates	51.84, 155.52, or 622.08 Mb/s (Nominal)

Specification (1310 nm Transmitter up to 2488.32 Mb/s)

Wavelength	1280 nm to 1330 nm (Typical 1310 nm)
Power Output	0.0 dBm to +3.0 dBm (Typical +1 dBm)
Line Coding	NRZ
Safety Class	Class 1, FDA 21 CFR Ch.1 1040.10 and EN 60825
Data Rates	51.84, 155.52, 622.08 or 2488.32 Mb/s (Nominal)

Specification (1550 nm Transmitter up to 622 Mb/s)

Wavelength	1480 nm to 1580 nm (Typical 1550 nm)
Power Output	-3.0 dBm to +2.0 dBm (Typical 0.0 dBm)
Line Coding	NRZ
Safety Class	Class 1, FDA 21 CFR Ch.1 1040.10 and EN 60825
Data Rates	51.84, 155.52, or 622.08 Mb/s (Nominal)

Specification (1550 nm Transmitter up to 2488.32 Mb/s)

Wavelength	1530 nm to 1570 nm (Typical 1550 nm)
Power Output	0.0 dBm to +3.0 dBm (Typical +1 dBm)
Line Coding	NRZ
Safety Class	Class 1, FDA 21 CFR Ch.1 1040.10 and EN 60825
Data Rates	51.84, 155.52, 622.08 or 2488.32 Mb/s (Nominal)

Performance Tests
Multirate Optical Interfaces

Specification (Receiver) up to 2488.32 Mb/s

Wavelength	1200 nm to 1600 nm
Maximum Input Power	-8 dBm (for BER of $1.0E^{-10}$)
Line Coding	NRZ
Sensitivity	-34 dBm (STM-0/1/4, OC-1/3/12) -28 dBm Minimum (STM-16, OC-48) (wavelength=1310/1550 nm, Modulation = 100%, Data= $2^{23}-1$, BER= $1.0E^{-10}$)
PMP Electrical Input	150mV pk-pk (Nominal) 51.84, 155.52 and 622.08 Mb/s only
PMP Impedance	Nominal 50Ω

Specification (Receiver) up to 622.08 Mb/s

Wavelength	1200 nm to 1600 nm
Maximum Input Power	-3 dBm (for BER of $1.0E^{-10}$)
Line Coding	NRZ
Sensitivity	-34 dBm (STM-0/1, OC-1/3) -28 dBm Minimum (STM-4, OC-12) (wavelength=1310/1550 nm, Modulation=100%, Data= $2^{23}-1$, BER= $1.0E^{-10}$)
PMP Electrical Input	150 mV pk-pk (Nominal), 51.84, 155.52 and 622.08 Mb/s only
PMP Impedance	Nominal 50Ω

NOTE

The rates available are dependent on the HP OmniBER 718 model and options fitted.

Description

The optical power output is measured on a power meter.

The receiver sensitivity is verified by attenuating the transmitter output and checking for no errors in back-to-back mode.

Performance Tests

Multirate Optical Interfaces

The Protected Monitor Point (PMP) functionality is verified by looping the HP OmniBER 718 Optical Output to the PMP input via an Optical Attenuator and Lightwave Converter, then checking for error-free operation.

Equipment Required

Power Meter	: HP 8153A
Power Meter Sensor Module	: HP 81536A
Oscilloscope	: HP 54520A
Lightwave Converter	: HP 11982A
Optical Attenuator	: HP 8157A
FC/PC Connector Interface	: HP 81000FI (Qty. 4)
Optical Cables (qty 2)	: HP 11871A
Adaptor (SMA to BNC)	: HP 1250-1787

WARNING

Safety precautions must be observed when handling the HP OmniBER 718 Optical Modules as these generate laser signals which can cause serious injury. The guidelines below must be followed:

Check the connector configuration of the 2.5 Gb/s Fiber Optic Interfaces. If non FC/PC connectors are fitted then remove them, then fit the FC/PC connector interface.

Check for any damage to the HP OmniBER 718 Fiber Optic Interface spring loaded aperture covers and connectors. Do not power up the instrument if in any doubt about the integrity of these connectors.

Make all connections to the HP OmniBER 718 Fiber Optic Interfaces before powering up the instrument.

Procedure

- 1 Switch on the HP OmniBER 718 and recall the DEFAULT SETTINGS as shown on page 3-4.

1310nm - Optical Power Output

- 2 Connect the HP OmniBER 718 Optical Out Port to the HP8153A.
Ensure all optical connectors are carefully cleaned before connections are made.
Ensure that all connections are tight and that the cable has no twists.

Performance Tests

Multirate Optical Interfaces

- 3 Setup the HP 8153A as follows:
 - a. Press **PARAM** key to display wavelength [λ]
 - b. Using **←**, **→**, **↑** and **↓** keys, set the wavelength to 1310nm.
 - c. Press **PARAM** key to display Time [t]
 - d. Using **←**, **→**, **↑** and **↓** keys, set the time to 200mS.
 - e. Press **PARAM** key to display REF.
 - f. Using **←**, **→**, **↑** and **↓** keys, set the REF to 0.000 dBm.
 - g. Press **PARAM** key to display CAL.
 - h. Using **←**, **→**, **↑** and **↓** keys, set the CAL to 0.000 dBm.
 - i. Press the **ZERO** key on the Power Meter to calibrate - the Power Meter is now ready.
- 4 Press **MODE** to select the Power Level measurement on the HP 8153A.
- 5 Press **TRANSMIT** **SDH** or **SONET**, and select SIGNAL [STM-0 OPT] or [OC-1].
- 6 Check the HP 8153A Power Meter reading is between 0 dBm and +3 dBm (Typically +1 dBm) for a 37718A. Or is between -3 dBm and +2dBm (Typically +0 dBm) for a 37718B/C.
- 7 Press **TRANSMIT** **SDH** or **SONET** and select SIGNAL [STM-1 OPT] or [OC-3].
- 8 Check the HP 8153A Power Meter reading is between 0 dBm and +3 dBm (Typically +1 dBm) for a 37718A. Or is between -3 dBm and +2dBm (Typically +0 dBm) for a 37718B/C.
- 9 **HP 37718A/B only.** Press **TRANSMIT** **SDH** or **SONET**, and select SIGNAL [STM-4 OPT] or [OC-12].
- 10 **HP 37718A/B only.** Check the HP 8153A Power Meter reading is between 0 dBm and +3 dBm (Typically +1 dBm) for a 37718A. Or is between -3 dBm and +2dBm (Typically +0 dBm) for a 37718B/C.
- 11 **HP 37718A only.** Press **TRANSMIT** **SDH** or **SONET** and select SIGNAL [STM-16 OPT] or [OC-48].
- 12 **HP 37718A only.** Check the HP 8153A Power Meter reading is between 0 dBm and +3 dBm (Typically +1 dBm) for a 37718A.

Optical Receiver Sensitivity

- 13 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 14 Set the Optical Attenuator to ATTEN 15 dB, WAVELENGTH 1310 nm; CAL=0; ENB ON. Connect the Optical Attenuator between the Power Meter and the HP OmniBER 718 Optical Out port (ensure that all connections are tight and

Performance Tests

Multirate Optical Interfaces

that the cable has no twists).

- 15 Press **TRANSMIT** **SDH** or **SONET** and select SIGNAL [STM-0 OPT] or [OC-1].
- 16 Adjust the Optical Attenuator to obtain a reading of -34 dBm on the Power Meter.
- 17 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 18 Disconnect the Optical Attenuator Output from the HP 8153A and connect to the HP OmniBER 718 Optical IN Port. Ensure all optical connectors are carefully cleaned before connections are made. Ensure that all connections are tight and that the cable has no twists.
- 19 Press **OTHER** then **SETTINGS CONTROL** and select TRANSMITTER AND RECEIVER [COUPLED].
- 20 Press **TRANSMIT** **SDH** or **SONET** and select SIGNAL [STM-0 OPT] or [OC-1].
- 21 Press **RESULTS** **TROUBLE SCAN** then **RUN/STOP** to start a measurement.
- 22 After 5 minutes check that NO TROUBLE is displayed on the **RESULTS** display.
- 23 Repeat steps 16 through 22, substituting SIGNAL [STM-1 OPT] or [OC-3] in steps 18 & 23.
- 24 **HP 37718A/B only.** Repeat steps 16 through 22, substituting SIGNAL [STM-4 OPT] or [OC-12] in steps 18 & 23. If 37718B/C then adjust the Optical Attenuator to obtain a reading of -28 dBm on the Power Meter
- 25 **HP 37718A only.** Repeat steps 16 through 22, substituting SIGNAL [STM-16 OPT] or [OC-48] in steps 18 & 23 and -28 dBm in step 19.


PMP Electrical Input

- 26 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 27 Disconnect the optical cable from the HP OmniBER 718 Optical IN port and connect to the HP 11982A Lightwave Converter input.
- 28 Connect the output from the Lightwave Converter to the Oscilloscope using the SMA/BNC adaptor and 50 Ω BNC cable.
- 29 Press **TRANSMIT** **SDH** or **SONET** and select SIGNAL [STM-0 OPT] or [OC-1].
- 30 Press **AUTOSCALE** on the Oscilloscope and adjust the Timebase and Range to obtain an STM-0/OC-1 waveform.

Performance Tests

Multirate Optical Interfaces

- 31 Measure the amplitude of the waveform using the Oscilloscope and adjust the Optical Attenuator until the amplitude is 150mV pk-pk.
- 32 Disconnect the output of the Lightwave Converter from the Oscilloscope and connect instead to the HP OmniBER 718 Optical Module Monitor input.
- 33 Press **RECEIVE** and set up the display as shown below.

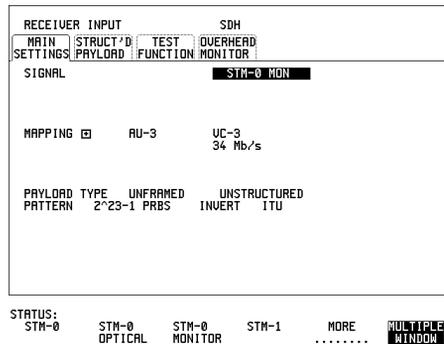

- 34 Press **RESULTS** **TROUBLE SCAN** then **RUN/STOP** to start the measurement.
- 35 After 5 minutes, check that NO TROUBLE is displayed on the **RESULTS** display. Press **RUN/STOP** to stop the measurement.
- 36 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 37 Repeat steps 28 to 36 but with [STM-1 OPT] or [OC-3] selected on the HP OmniBER 718 **TRANSMIT** and **RECEIVE** displays.
- 38 Recall the HP OmniBER 718 DEFAULT SETTINGS as shown on page 3-4.
- 39 Repeat steps 28 to 36 but with [STM-4 OPT] or [OC-12] selected on the HP OmniBER 718 **TRANSMIT** and **RECEIVE** displays.

Procedure 1550 nm - Optical Power Output

- 40 Repeat steps 1 through 12 substituting 1550nm for 1310nm.

Optical Receiver Sensitivity

- 41 Repeat Steps 13 through 25 substituting 1550nm for 1310nm.

Performance Tests
Multirate Optical Interfaces

Performance Tests
Performance Test Record

Performance Test Record

HP OmniBER 718	
Multirate Communications Performance Analyzer	
Location:	Serial No.:
Tested by:	Options:
Temperature:	Certified by:
Humidity:	Date:

Note the test steps applicable are dependent on the instrument options and bit rates available.
 Enter N/A if a test does not apply for your instrument

Performance Test Record

Page No.	Test Description		Result		
			Min	Actual	Max
3-5	Self Test				
3-6	Step 3	Confidence Tests		Pass/Fail	
3-7	Step 4	All Tests		Pass/Fail	
3-8	Step 3	1550 nm Tests		Pass/Fail	
3-9	Step 3	DCC Tests		Pass/Fail	
3-10	PDH/DSn Internal Transmitter Clock Accuracy & Offset				
3-11	Step 4:	2 Mb/s	1.023995 MHz		1.024005 MHz
	Step 6:	2 Mb/s +50 ppm	1.0240465 MHz		1.0240555 MHz
3-12	Step 8:	2 Mb/s -50 ppm	1.023944 MHz		1.023953 MHz
	Step 10:	8 Mb/s	4.223981 MHz		4.224019 MHz
	Step 12:	8 Mb/s +30 ppm	4.2241075 MHz		4.2242915 MHz
	Step 14:	8 Mb/s -30 ppm	4.223854 MHz		4.223892 MHz
3-12	Step 16:	34 Mb/s	17.18389227 MHz		17.1840774 MHz

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Result		
			Min	Actual	Max
	Step 18:	34 Mb/s +20ppm	17.184266 MHz		17.184421 MHz
	Step 20:	34 Mb/s -20ppm	17.183579 MHz		17.183734 MHz
3-13	Step 22:	34 Mb/s +100ppm	17.185641 MHz		17.185796 MHz
	Step 24:	34 Mb/s -100ppm	17.182205 MHz		17.182359 MHz
	Step 26:	140 Mb/s	69.6316865 MHz		69.6323185 MHz
	Step 28:	140 Mb/s +15ppm	69.632731 MHz		69.633358 MHz
	Step 30:	140 Mb/s -15ppm	69.630642 MHz		69.631269 MHz
	Step 33:	1.544 Mb/s	1.543993 MHz		1.544007 MHz
3-14	Step 35:	1.544 Mb/s +32ppm	1.544042 MHz		1.544056 MHz
	Step 37:	1.544 Mb/s -32ppm	1.543944 MHz		1.543958 MHz
	Step 40:	44.736 Mb/s	44.735799 MHz		44.736201 MHz
	Step 42:	44.736 Mb/s +20ppm	44.736693 MHz		44.737096 MHz
	Step 44:	44.736 Mb/s -20ppm	44.734904 MHz		44.735307 MHz
3-15	PDH/DSn Transmitter Output				
		139.264Mb/s (E4)			
3-17	Step 7:	All 1's Pulse		Pass/Fail	
	Step 8:	Pulse amplitude		Pass/Fail	
3-18	Step 12:	All 0's Pulse		Pass/Fail	
	Step 13:	Pulse amplitude		Pass/Fail	
		34.368Mb/s (E3)			
3-20	Step 7:	+ve Pulse		Pass/Fail	
	Step 8:	+ve Pulse amplitude		Pass/Fail	
3-21	Step 12:	-ve Pulse		Pass/Fail	
	Step 13:	-ve Pulse amplitude		Pass/Fail	
		8.448Mb/s (E2)			
3-22	Step 7	+ve Pulse		Pass/Fail	

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Min	Result	Max
				Actual	
	Step 8:	+ve Pulse amplitude		Pass/Fail	
3-23	Step 12:	-ve Pulse		Pass/Fail	
	Step 13:	-ve Pulse amplitude		Pass/Fail	
		2.048Mb/s (E1)			
3-25	Step 7:	+ve Pulse		Pass/Fail	
	Step 8:	+ve Pulse amplitude		Pass/Fail	
	Step 12:	-ve Pulse		Pass/Fail	
3-26	Step 13:	-ve Pulse amplitude		Pass/Fail	
		44.736Mb/s (DSX3)			
3-27	Step 7:	+ve Pulse		Pass/Fail	
	Step 8:	+ve Pulse amplitude		Pass/Fail	
3-28	Step 12:	-ve Pulse		Pass/Fail	
	Step 13:	-ve Pulse amplitude		Pass/Fail	
	Step 14:	High amplitude		Pass/Fail	
	Step 15:	Low amplitude		Pass/Fail	
		1.544Mb/s (DSX1)			
3-30	Step 8:	+ve Pulse		Pass/Fail	
	Step 9:	+ve Pulse amplitude		Pass/Fail	
3-31	Step 13:	-ve Pulse		Pass/Fail	
	Step 14:	-ve Pulse amplitude		Pass/Fail	
	Step 15:	Low amplitude		Pass/Fail	
3-32	PDH/DSn Receiver Equalization				
3-33	Step 6:	139.264 Mb/s (E4)		Pass/Fail	
3-34	Step 11:	34.368 Mb/s (E3)		Pass/Fail	

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Min	Result	Max
				Actual	
3-35	Step 16:	44.736 Mb/s (DS3)		Pass/Fail	
3-36	Step 21:	8.448 Mb/s (E2)		Pass/Fail	
3-37	Step 26:	2.048 Mb/s (E1)		Pass/Fail	
3-38	Step 31:	1.544 Mb/s (DS1)		Pass/Fail	
3-39	PDH/DSn Receiver Monitor Levels				
		2.048Mb/s (E1)			
3-41	Step 5:	20 dB		Pass/Fail	
	Step 10:	20 dB & Equalization		Pass/Fail	
	Step 14:	26 dB & Equalization		Pass/Fail	
3-42	Step 18:	26 dB		Pass/Fail	
	Step 22:	30 dB		Pass/Fail	
	Step 26:	30 dB & Equalization		Pass/Fail	
		8.448Mb/s (E2)			
	Step 27:	20 dB		Pass/Fail	
	Step 27:	20 dB & Equalization		Pass/Fail	
	Step 27:	26 dB & Equalization		Pass/Fail	
	Step 27:	26 dB		Pass/Fail	
	Step 27:	30 db		Pass/Fail	
	Step 27:	30 dB & Equalization		Pass/Fail	
		34.368Mb/s (E3)			
3-42	Step 28:	20 dB		Pass/Fail	
3-42	Step 28:	20 dB & Equalization		Pass/Fail	
	Step 28:	26 dB & Equalization		Pass/Fail	
	Step 28:	26 dB		Pass/Fail	
		139.264Mb/s (E3)			
	Step 29:	20 dB		Pass/Fail	

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Result		
			Min	Actual	Max
	Step 29:	20 dB & Equalization		Pass/Fail	
	Step 29:	26 dB & Equalization		Pass/Fail	
	Step 29:	26 dB		Pass/Fail	
		1.544Mb/s (DS1)			
3-43	Step 30:	20 dB		Pass/Fail	
	Step 30:	20 dB & Equalization		Pass/Fail	
	Step 30:	26 dB & Equalization		Pass/Fail	
	Step 30:	26 dB		Pass/Fail	
	Step 30:	30 db		Pass/Fail	
	Step 30:	30 dB & Equalization		Pass/Fail	
		44.736Mb/s (E3)			
	Step 31:	20 dB		Pass/Fail	
	Step 31:	20 dB & Equalization		Pass/Fail	
	Step 31:	26 dB & Equalization		Pass/Fail	
	Step 31:	26 dB		Pass/Fail	
3-44	External Mux/Demux				
3-48	Step 9:	2 Mb/s Bit & Code EC		Pass/Fail	
	Step 10:	2 Mb/s Bit Error Add		Pass/Fail	
3-49	Step 15:	+ve Mask 2 Mb/s		Pass/Fail	
	Step 16:	+ve Amp 2 Mb/s		Pass/Fail	
3-50	Step 20	-ve Mask 2 Mb/s		Pass/Fail	
3-50	Step 21:	-ve Amp 2 Mb/s		Pass/Fail	
	DS-1 Mux and Demux				
	Step 1:	DS-1 Bit & Code EC		Pass/Fail	
	Step 1:	DS-1 Bit Error Add		Pass/Fail	
3-51	Step 6:	+ve Pulse Mask DS-1		Pass/Fail	
3-52	Step 7:	+ve Pulse Amp DS-1		Pass/Fail	

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Min	Result	Max
				Actual	
	Step 11	-ve Pulse Mask DS-1		Pass/Fail	
3-53	Step 12:	-ve Pulse Amp DS-1		Pass/Fail	
3-54	PDH Frequ. Measurement and Looped Clock				
3-56	Step 8:	2Mb/s frequency	2.047991 MHz		2.048009 MHz
	Step 9:	Offset (0 ppm)	-4.5 ppm		+4.5 ppm
	Step 10:	Frequency+100 ppm	2.048194 MHz		2.048214 MHz
3-57	Step 11:	Offset +100 ppm	+95.5 ppm		+104.5 ppm
	Step 12:	Frequency-100 ppm	2.047786 MHz		2.047806 MHz
	Step 13:	Offset -100 ppm	-95.5 ppm		-104.5 ppm
	Step 13:	Frequency Counter		Pass/Fail	
	Step 14:	8Mb/s 0 ppm	-4.5 ppm		+4.5 ppm
	Step 14:	8Mb/s -100 ppm	-95.5 ppm		-104.5 ppm
	Step 14:	8Mb/s +100 ppm	+95.5 ppm		+104.5 ppm
	Step 14:	34 Mb/s 0 ppm	-4.5 ppm		+4.5 ppm
	Step 14:	34 Mb/s -100 ppm	-95.5 ppm		-104.5 ppm
	Step 14:	34 Mb/s +100 ppm	+95.5 ppm		+104.5 ppm
	Step 14:	40 Mb/s 0 ppm	-4.5 ppm		+4.5 ppm
	Step 14:	140 Mb/s -100 ppm	-95.5 ppm		-104.5 ppm
	Step 14:	140 Mb/s +100 ppm	+95.5 ppm		+104.5 ppm
3-57	Step 14:	1.544 Mb/s 0 ppm	-4.5 ppm		+4.5 ppm
	Step 14:	1.544 Mb/s -100 ppm	-95.5 ppm		-104.5 ppm
	Step 14:	1.544 Mb/s +100 ppm	+95.5 ppm		+104.5 ppm
	Step 14:	44.736 Mb/s 0 ppm	-4.5 ppm		+4.5 ppm
	Step 14:	44.736Mb/s -100 ppm	-95.5 ppm		-104.5 ppm
	Step 14:	44.736Mb/s+100 ppm	+95.5 ppm		+104.5 ppm

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Min	Result	Max
				Actual	
3-58	SDH/SONET Transmitter Clock Accuracy				
	Step 4:	Frequency	51.839670 MHz		51.840230 MHz
3-59	External Clock/Data Reference Inputs & Clock Reference Output				
3-61	Step 7:	2Mb/s Clock		Pass/Fail	
	Step 9:	Ref Clock Out		Pass/Fail	
3-62	Step 16:	2 Mb/s Data		Pass/Fail	
	Step 21:	2 Mb/s Data Balanced		Pass/Fail	
	Step 25:	Rx Data Clock Loss		Pass/Fail	
	Step 28:	Rx Data Clock Gain		Pass/Fail	
	Step 30:	10 MHz Clock Loss		Pass/Fail	
3-63	Step 33:	10 MHz Clock Gain		Pass/Fail	
	Step 35:	BITS Clock Loss		Pass/Fail	
	Step 38:	BITS Clock Gain		Pass/Fail	
	Step 41:	64 kb/s Clock Loss		Pass/Fail	
	Step 42:	64 kb/s Clock Gain		Pass/Fail	
3-64	SDH/SONET Freq. Offsets				
	Step 5:	Clock Loss		Pass/Fail	
3-65	Step 10:	0 ppm		51.84MHz	
3-65	Step 11:	-999 ppm	51.7882108 MHz		51.7882129 MHz
	Step 11:	-100 ppm	51.8348149 MHz		51.8348171MHz
	Step 11:	-66 ppm	51.8365464 MHz		51.8365485 MHz
	Step 11:	+33 ppm	51.8417252 MHz		51.8417273 MHz
	Step 11:	+100 ppm	51.8451829 MHz		51.8451851MHz
	Step 11:	+999 ppm	51.8917871 MHz		51.8917892 MHz

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Result		
			Min	Actual	Max
3-66	STM-0/STS-1 Transmitter Output Waveshape				
3-67	Step 6:	+ve Pulse		Pass/Fail	
3-68	Step 7:	+ve Pulse Amp		Pass/Fail	
	Step 11:	-ve Pulse		Pass/Fail	
3-69	Step 12:	-ve Pulse Amp		Pass/Fail	
	Step 13:	High amplitude		Pass/Fail	
	Step 14:	Low Amplitude		Pass/Fail	
3-70	STM-1/STS-3 Transmitter Output Waveshape				
3-73	Step 8:	All 1's Pulse		Pass/Fail	
	Step 9:	Pulse Amp	450 mV pk		550 mV pk
	Step 13:	All 0's Pulse		Pass/Fail	
3-74	Step 14:	Pulse Amp	450 mV pk		550 mV pk
3-75	SDH/SONET Receiver Equalization				
3-76	Step 5:	STM-0/STS-1		Pass/Fail	
3-77	Step 10:	STM-1/STS-3		Pass/Fail	
3-78	SDH/SONET Receiver Monitor Levels				
		STM-0/STS-1			
3-80	Step 5:	20dB		Pass/Fail	
	Step 9:	20dB + Equalization		Pass/Fail	
	Step 14:	26dB + Equalization		Pass/Fail	
3-81	Step 18:	26dB		Pass/Fail	
		STM-1/STS-3			
	Step 20:	20dB		Pass/Fail	
	Step 20:	20dB + Equalization		Pass/Fail	

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Result		
			Min	Actual	Max
	Step 20:	26dB + Equalization		Pass/Fail	
	Step 20:	26dB		Pass/Fail	
3-82	Multirate Optical Interface				
		Power 1310 nm			
3-85	Step 6:	STM-0/OC-1	0 dBm (37718A) -3 dBm (37718B/C)		+3 dBm (37718A) +2 dBm (37718B/C)
	Step 8:	STM-1/OC-3	0 dBm (37718A) -3 dBm (37718B/C)		+3 dBm (37718A) +2 dBm (37718B/C)
	Step 10:	STM-4/OC-12	0 dBm (37718A) -3 dBm (37718B/C)		+3 dBm (37718A) +2 dBm (37718B/C)
	Step 12:	STM-16/OC-48	0 dBm (37718A)		+3 dBm (37718A)
		Sensitivity 1310 nm			
3-86	Step 22:	STM-0/OC-1		Pass/Fail	
	Step 23:	STM-1/OC-3		Pass/Fail	
	Step 24:	STM-4/OC-12		Pass/Fail	
	Step 25:	STM-16/OC-48		Pass/Fail	
		PMP input			
3-87	Step 35:	STM-0/OC-1		Pass/Fail	
	Step 37:	STM-1/OC-3		Pass/Fail	
	Step 39:	STM-4/OC-12		Pass/Fail	
		Power 1550nm			
3-87	Step 40:	STM-0/OC-1	0 dBm (37718A) -3 dBm (37718B/C)		+3 dBm (37718A) +2 dBm (37718B/C)
	Step 40:	STM-1/OC-3	0 dBm (37718A) -3 dBm (37718B/C)		+3 dBm (37718A) +2 dBm (37718B/C)
	Step 40:	STM-4/OC-12	0 dBm (37718A) -3 dBm (37718B/C)		+3 dBm (37718A) +2 dBm (37718B/C)
	Step 40:	STM-16/OC-48	0 dBm (37718A)		+3 dBm (37718A)
		Sensitivity 1550nm			

Performance Tests
Performance Test Record

Performance Test Record , continued

Page No.	Test Description		Result		
			Min	Actual	Max
	Step 41:	STM-0/OC-1		Pass/Fail	
	Step 41:	STM-1/OC-3		Pass/Fail	
	Step 41:	STM-4/OC-12		Pass/Fail	
	Step 41:	STM-16/OC-48		Pass/Fail	

4

Terms

This section contains a table of the current (and earlier) ETSI terms and the ANSI equivalents.

ETSI/ANSI Conversion and Equivalent Terms

Introduction

The terminology used on the instrument display can be ETSI (SDH) or ANSI (SONET) terminology. Refer to the table given in this chapter for an explanation of equivalent SDH/SONET terms.

ETSI: European Telecommunications Standards Institute.

ANSI: American National Standards Institute.

ETSI Term	ANSI Term
AU-3	STS-1 SPE + H1, H2, H3
AU-4	STS-3c SPE + H1, H2, H3
BIP (Bit Interleaved parity)	CV (Code Violation)
High Order Path (HP / HO)	STS Path
I-n Intra Office, (n=STM-n level)	Intermediate Reach (IR)
L-n.1 or L-n.2 long haul	LR long reach
Low Order Path (LP / LO)	VT Path
LP-REI	REI-V
M.S.P	A.P.S
Multiplexer Section (MS)	Line
Multiplexer Section Protection	Automatic Protection Switching
MS-AIS	Line AIS / AIS-L
MS-BIP	Line CV / CV-L

Terms

ETSI Term	ANSI Term
MS-DCC	Line DCC / DCC-L
MS-REI	Line FEBE / REI-L
MS-RDI	Line FERF / RDI-L
Multiplexer Section Overhead	Line Overhead
Network Node Interface	Line Interface
OOF	SEF (severely errored frame defect)
Path AIS / AU-AIS	AIS-P
Path REI / HP REI	REI-P
Path FERF / HP RDI	RDI-P
Path IEC / AU-IEC	IEC-P
Path Overhead	Path Overhead
Regenerator	Repeater
Regenerator Section (RS)	Section
Regenerator Section Overhead	Section Overhead
Remote Alarm Indicator	RAI
RS-DCC	Section DCC (DCC-S)
Section Overhead (SOH)	Transport Overhead (TOH)
S-n.1 or S-n.2 short haul	Short Reach (SR)
SOH	TOH
STM-m	OC-n / STS-n (where $m = n \div 3$ for $m \geq 1$)
STM-0	STS-1
STM-1	OC3c / STS-3c
STM-4	OC-12 / STS-12
STM-16	OC-48 / STS-48
Tributary Unit (TU)	Virtual Tributary (VT)

Terms

ETSI Term	ANSI Term
TU	VT
TU-11	VT 1.5
TU-12	VT 2
TU-2	VT 6
TU-3	NONE
TU BIP	VT BIP (CV-V)
TU RDI / LP-RDI	RDI-V
TUG	VT Group
TUG2	VT Group (12 columns)
TUG3	VT Group (86 columns)
TU multiframe	VT superframe
TU PATH AIS	VT AIS (AIS-V)
VC	SPE
VC4	STS3C SPE
Virtual Container (VC)	Synchronous Payload Envelope (SPE)

NOTE: VC is an ETSI abbreviation for Virtual Container and an ETSI/ANSI abbreviation for (ATM) Virtual Channel. The context of VC must therefore be taken into account when converting between standards.

5

Self Test Overview

Self Tests

This section gives an overview of the Self Tests and their function.

There are several Self Test selections. Some providing overall functional tests and others provide specific measurement hardware/functions tests.

Overall Function Self Tests

Confidence Test (test time - < 5 minutes depending on options)

Provides a quick verification of the main instrument functions using external back-to-back loopback of the instrument Transmit/Receive sections. See the Table below for a list of the subtests, and Figure 5-1 for the external loopback cabling required for this test. Use this test to provide a quick operational verification.

<u>Subtest</u>	<u>Test Function</u>
1	PDH 140 Mb/s Structured 64 kb/s
2	PDH 2 Mb/s 120 ohm balanced
3	PDH 34 Mb/s Structured 64 kb/s
4	PDH DS1, D4 Structured 64 kb/s
5	SDH, STM-0e Test
6	SDH, STM-0e Test
7	SDH, STM-1e Test
8	SDH, STM-1o Test
9	SDH, STM-4o Test
10	SDH, STM-16o Test
11	OPT 2xx Jitter Test, PDH 34 Mb/s
12	OPT 2xx Jitter Test, SDH 622 Mb/s

Self Tests

All Tests (test time - up to 1 hour depending on options)

Provides an extensive back-to-back verification test of the instrument operation. The test uses much of the specific function tests, performing the appropriate subtest depending on options fitted. Test are run as follows.

CPU test

CONFIDENCE test

PDH test

BER test (Note does not perform DCC port test)

See Tables for each of these tests for a list of the subtests and Figure 5-1 for the loopback cabling required for this test. Note a Formatted floppy disk is required as the CPU test is run as part of All Tests selection.

Use this test to provide a comprehensive operational verification.

Specific Measurement Hardware/Function Tests

CPU Tests (test time - approximately 2 minutes)

Provides a quick test of the Main and Front Panel processors. No external cabling is required, but formatted floppy disk must be installed.

<u>Subtest</u>	<u>Test Function</u>
1	Flash ROM CRC checks
2	Ram Test
3-7	Not used
8	In-Lid Printer present check, (if option 602 fitted)
9	Not used
10	Floppy disk write/read
11	Not used
12-16	Front Panel processor checks

Self Test Overview

Self Tests

PDH Test (test time- approximately 20 minutes)

Provides comprehensive test of the PDH Transmit/Receive sections. Note this test is run as part of ALL TESTS. The Subtests used are dependent on PDH option.

<u>Subtest</u>	<u>Test Function</u>
1-7	Line Code Tests (140/34/8/2 MHz Unable 75 ohm)
8-9	Line Code Tests (2 MHz Balanced 120 ohm)
10-21	Frequency Offset (140/34/8/2 MHz)
22-36	Error Add/Detect (34/2 MHz)
37-44	Framing (140/2 MHz)
45-53	Structured Payloads (140/34/8 MHz)
54-63	Patterns (140/34/8 MHz)
64	Drop/Insert (2 MHz)
65-72	Round Trip Delay (64 kb/s)
73-82	Not used
83-86	Line Code Tests (DS3/DS1 Unable 75 ohm)
87-88	Line Code Tests (DS1 Balanced 110 ohm)
89-94	Frequency Offset (DS3/DS1)
95-112	Error Add/Detect (DS3/DS1)
113-120	Framing (DS3/DS1)
121-130	Structured Payloads (DS3/DS1)
134-140	Patterns (DS3/DS1)
141	Drop/Insert (DS1)
142-145	Round Trip Delay
146-148	DS1 Unbalanced Tx/Rx tests
149-150	DS3 Unbalanced Tx/Rx tests

Self Tests

BER Test (test time- approximately 20 minutes)

These tests perform extensive test of the SDH/SONET Electrical and Optical Transmit/Receive sections. Note this test is run as part of ALL TESTS with the exception of Subtest 83, DCC port test.

<u>Subtest</u>	<u>Test Function</u>
1	STM-16 MUX/DEMUX Internal Loopback
2-4	STM-0e Pulse Shape
5-8	Basic STM-0o Tx/Rx Test
7-8	Basic STM-1e Tx/Rx Test
9-10	Basic STM-1o Tx/Rx Test
11-12	Basic STM-4o Tx/Rx Test
13-14	Basic STM-16o Tx/Rx Test
15-17	STM-4o Frequency Measurement
18	STM-16o Frequency Measurement
19-20	Clock Reference Source
21-22	Optical Power Measurement
23	Overhead Byte Defaults [part 1]
24	Overhead Byte Defaults [part 2]
25	STM16o J0 Path Trace Message
26	J1 Path Trace Message
27	J2 Path Trace Message
28-35	SDH Error Add[RATE]/Detection
36-44	SDH Single Error Add/Detection
45	STM-16o Entire Frame Error Add/Detect
46	A1A2 Frame Error Add
47-49	PDH Payload Error Add[RATE]/Detection
50-52	PDH Payload Single Error Add/Detection
53-67	Alarm Generation/Detection
68-69	OOB Alarm Generation/Detection

Self Test Overview

Self Tests

70	TU-3/TU12 Mixed Payload Test
71	TU-12/TU-3 Mixed Payload Test
72	TU-3/TU-11 Mixed Payload Tests
73	TU-11/TU-3 Mixed Payload Tests
74-75	AU New Pointer Test
76-77	AU Frequency Offset Pointer Moves
78-79	TU Frequency Pointer Moves
80-81	STM-16o 140 Mb/s Payload VC Offset Test
82	TU-3 Background Pattern Test
83	DCC Port Test
84-87	Stress Test
88-99	Service Disruption Test

Self Test Overview

Self Tests

Long Gating test (test time- approximately 6 Hours)


This test performs an extended gating check of each SDH/SONET Optical rate to confirm error free operation. Test time at each rate is sufficient to ensure that the error ratio is less than 1 in 10^{12} . The test does NOT form part of ALL TESTS.

<u>Subtest</u>	<u>Test Function</u>
1	Tx/Rx STM-0o with Bulk 2^{23} Payload
2	Tx/Rx STM-1o with Bulk 2^{23} Payload
3	Tx/Rx STM-4o with Bulk 2^{23} Payload
4	Tx/Rx STM-16o with Bulk 2^{23} Payload

Self Test Overview

Self Tests

Loopbacks Required by Each Self Test

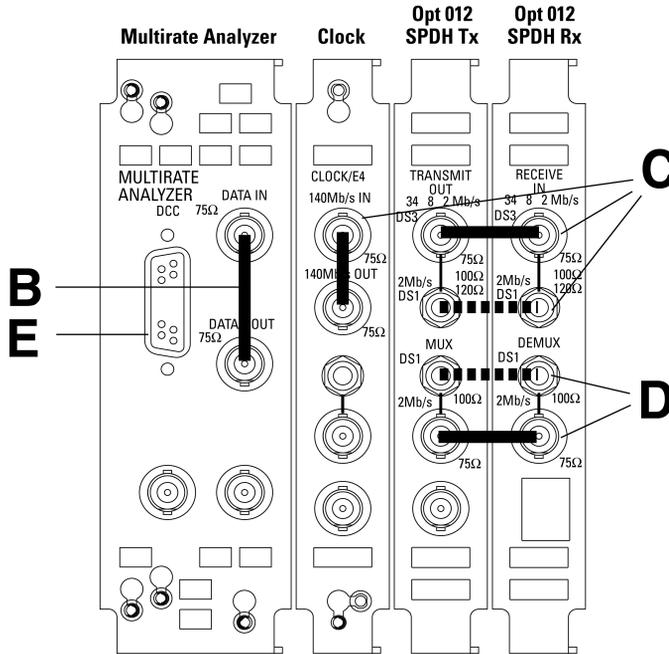

**HP 37718B/C communications performance analyzer
155M electrical tester**

Minimum loopbacks required by each test

TEST	A	B	C	D	E	F
Conf		X	X			
All		X	X	X		X
CPU						X
PDH			X	X		
BER		X			X	
Jitter		X	X			
Long gating						

- HP 15552A BNC 75Ω loopback
- HP 15670A Bantam 110Ω loopback
- HP 4545A 3m fiber optic cable FC/PC


Note 1:
A formatted floppy disk *must* be fitted into the disk drive before running 'All' or 'CPU' self tests.

Note 2:
A 15 dB optical attenuator (HP 4546A) *must* be fitted at the optical *output* port.

Note 3:
If running BER self tests, a loopback *must* be connected to the DCC port (see P3-9).

Self Test Overview

Self Tests

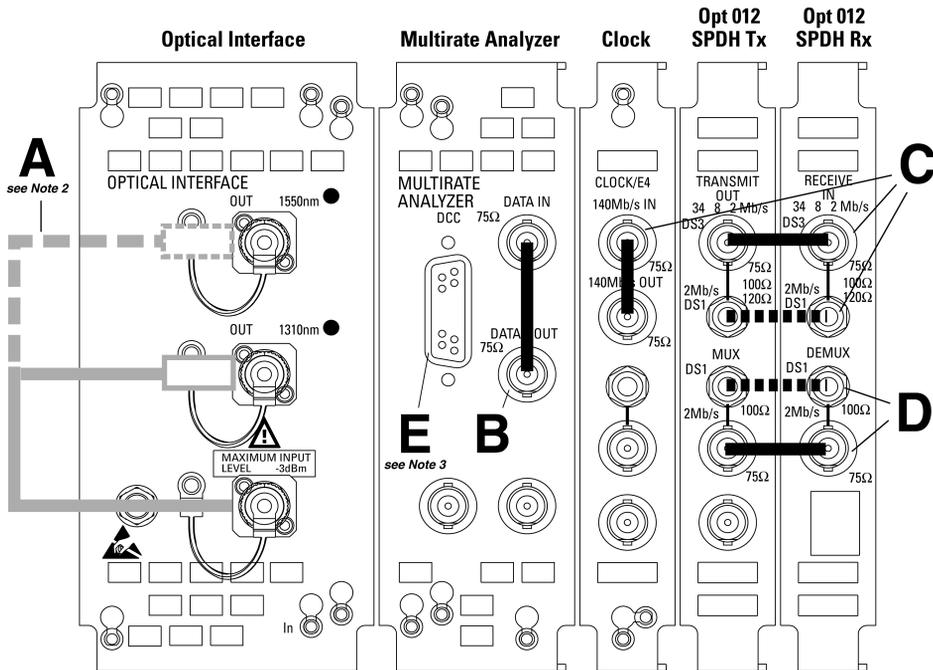

**HP 37718B/C communications performance analyzer
622M/155M dual wavelength tester**

Minimum loopbacks required by each test

TEST	A	B	C	D	E	F
Conf	X	X	X			
All	X	X	X	X		X
CPU						X
PDH			X	X		
BER	X	X			X	
Jitter	X	X	X			
Long gating	X					

- HP 15552A BNC 75Ω loopback
- HP 15670A Bantam 110Ω loopback
- HP 4545A 3m fiber optic cable FC/PC


Note 1:
A formatted floppy disk *must* be fitted into the disk drive before running 'All' or 'CPU' self tests. **F**

Note 2:
A 15 dB optical attenuator (HP 4546A) *must* be fitted at the optical *output* port.

Note 3:
If running BER self tests, a loopback *must* be connected to the DCC port (see P3-9).

Self Test Overview

Self Tests

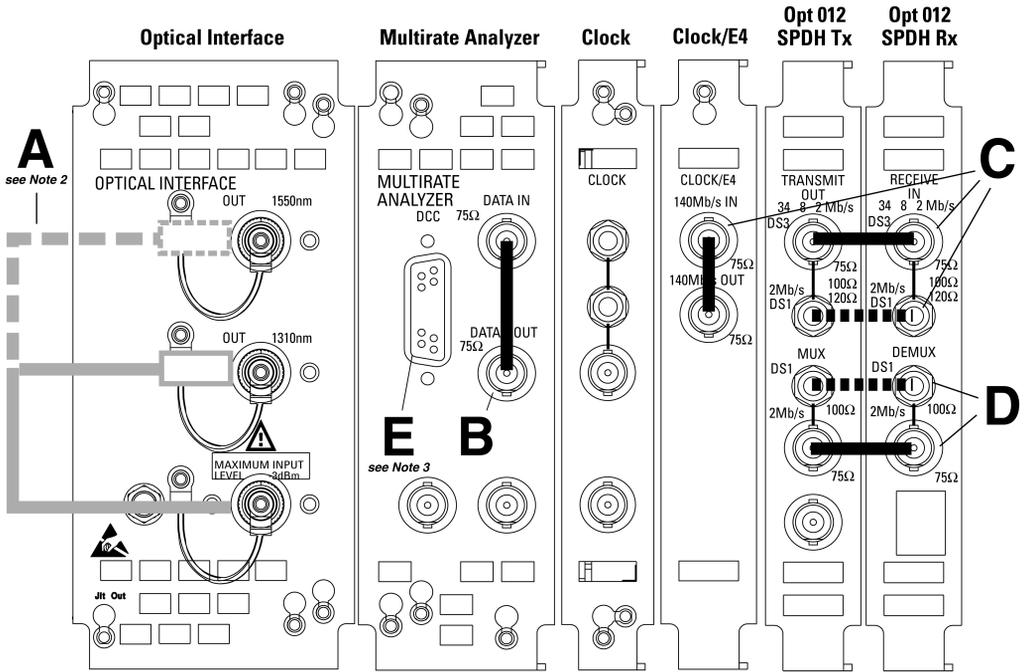

**HP 37718A communications performance analyzer
2.5 Gb/s dual wavelength tester**

Minimum loopbacks required by each test

TEST	A	B	C	D	E	F
Conf	X	X	X			
All	X	X	X	X		X
CPU						X
PDH			X	X		
BER	X	X			X	
Jitter	X	X	X			
Long gating	X					

- HP 15552A BNC 75Ω loopback
- HP 15670A Bantam 110Ω loopback
- HP 4545A 3m fiber optic cable FC/PC

Note 1:
A formatted floppy disk *must* be fitted into the disk drive before running 'All' or 'CPU' self tests. **F**

Note 2:
A 15 dB optical attenuator (HP 4546A) *must* be fitted at the optical *output* port.

Note 3:
If running BER self tests, a loopback *must* be connected to the DCC port (see P3-9).

Self Test Overview

Self Tests

Self Test Errors

The Tests will halt if a Self Test Error is detected. A message indicating the test point being run and error detected is displayed. Check all loopback connections and re-run the test. If the problem persists and contact your local HP Service Office or representative. Tests should only performed in a stable ambient environment where the instrument will not be disturbed during test.

The Self Test Error code numbering uses the following numeric format.

First Number indicates the Test being run.

CPU	1xxx
CONFIDENCE	2xxx
PDH	3xxx (for Subtests < 100), 18xxx (for Subtests 100+)
BER	4xxx
LONG GATING	6xxx

Note ALL TESTS uses the number from the tests it calls.

The next digits indicate the Subtest, e.g. 415x, is Subtest 15 of Test 4 (BER).

(where subtests are >99 the numbering restarts)

The last digit indicates the error type. In general these are -

- 1 = Loss of Signal
- 2 = specific for subtest
- 3 = test result too low
- 4 = test result too high
- 5 = loss of frame sync
- 6 = loss of pointer sync
- 7 = loss of pattern sync

The error codes are accompanied by appropriate error messages.

6

Option Structure/Module Configuration

Introduction

The HP OmniBER 718 provides SDH/SONET test capability, a choice of 1310 nm and 1550 nm Optics, and BER testing over the range from PDH rates up to 2.488 Gb/s.

HP OmniBER 718 Mainframe

HP 37718A provides SDH/SONET test capability at 2.5 Gb/s and below.

HP 37718B provides SDH/SONET test capability at 622 Mb/s and below.

HP 37718C provides SDH/SONET test capability at 155 Mb/s and below.

PDH/Dsn Option

Option 012 provides E1, E2, E3, E4, DS1, and DS3 rates.

SDH/SONET Options

Option 001 provides SDH only.

Option 002 provides SDH/SONET.

OPTICS Options


Option 104 provides 1310 nm Optics.

Option 105 provides 1550 nm Optics.

Option 106 provides 1310/1550 nm Dual Optics.

Option Structure/Module Configuration

37718A/B/C Multirate BER configurations - Options 104/105/106

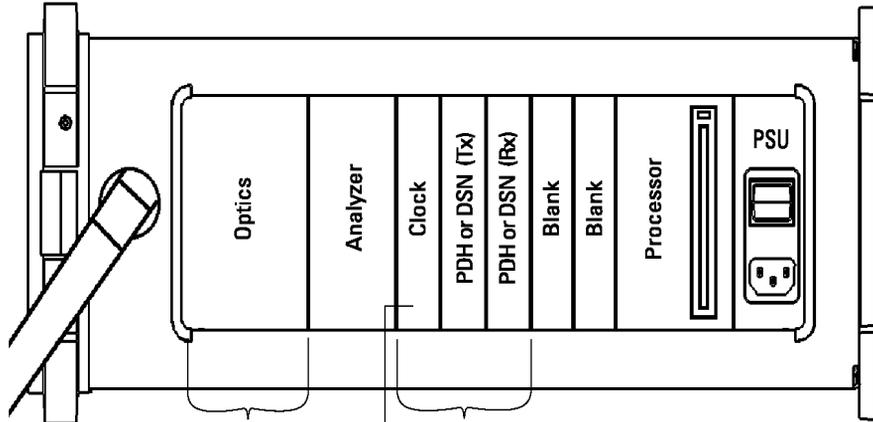

Opt 104 : 1310 nm

Opt 105 : 155 nm

Opt 106 : 1310 + 1550 nm

Opt 010 : PDH 2/8/34/140 rates

Opt 011 : DS_n DS1/DS3/E1/E3

Opt 012 : PDH 2/8/34/140/DS1/DS3

Opt 013 : DS_n T-carrier + DS1/DS3/2/8/34

If HP 37718A, then two clock cards are fitted to provide clock up to 2.5 Gb/s.

If HP 37718B/C, then clock card provides E4 data and clock.

Index

A

Accessories

- Connection 2-11

Alternative External MTS Clock 3-64

Assistance 1-3

Australian EMC Regulations

- Compliance with 1-10

C

Certification 1-3

Cleaning 1-8

- Instrument 1-8

- Optical Connectors 1-8

CLOCK TRIGGER 2-8

Compliance, Statement of 1-10

Connecting

- Accessories 2-11

- ESD Precautions Necessary 2-6

- To the Network 2-6

- To the Power Supply 2-4

Connectors

- Electrical Interface 2-6

- Optical Interface 2-9

D

DEMUX 2 Mb/s 75 ohm Connector 2-7

DEMUX DS1 100 ohm Connector 2-7

Dimensions and Weight 1-5

DS1 100 ohm, 2Mb/s 120 ohm IN Connector 2-6

DS1 100 ohm, 2Mb/s 120 ohm OUT 2-7

DS3, 2Mb/s, 34Mb/s 75 ohm IN Connector 2-6

DS3, 2Mb/s, 34Mb/s 75 ohm OUT Connector 2-6

E

Electrical Interface Connectors 2-6

Electromagnetic Compatibility 1-11

Environment

- Operating 2-2

- Storage and Shipment 1-4

ESD Precautions

Index

For the Service Engineer 2-6, 2-14

External 2Mb/s Mux/Demux 3-44

External MTS Clock 3-59

F

Fuse Replacement 2-3

Fuses 2-3

G

General Purpose Interface Bus 2-12

GPIB 2-12

H

HANDSET Connector 2-11

HP-IB

Address Selection 2-13

HP-IB Address 2-13

HP-IB Connection 2-12

I

Inspection, Initial 2-1

Instrument Cleaning 1-8

Instruments Covered By Manual 1-4

Internal SDH Transmitter Clock 3-58

L

Laser apertures

Location 2-10

LID Connector 2-11

Lifting/Carrying the Instrument 1-6

Location of Laser Apertures 2-10

M

Maintenance by the Operator 1-8

MUX 2 Mb/s 75 ohm Connector 2-7

MUX Connector 2-7

MUX DS1 100 ohm Connector 2-7

N

Noise Declaration (German) 1-10

O

Operators Maintenance 1-8

Optical Connector Cleaning 1-8

OPTICAL IN Connector 2-10

Index

Optical Interface Connectors 2-9

OPTICAL OUT Connector 2-10

P

PDH Frequency Measurement and Looped Clock 3-54, 3-57

PDH Receiver Equalization 3-32, 3-75

Performance Test Record 3-89

Power Cord 2-5

Power Requirements 2-3

Power Supply Connection 2-4

Precautions

 ESD when connecting 2-6

Precautions for the Service Engineer 2-14

Preparation for Use 2-3

Printer HP-IB, RS232, PARALLEL ONLY Connector 2-11

R

Recall Default Settings 3-4

RECEIVER 2,8,34,140 IN 2-6

Recommended Test Equipment 3-5

REF OUT 2-7

Remote Control HP-IB, RS232, 10 BASE -T Connector 2-11

Repackaging 1-4

Responsibilities of the Customer 1-2

Restricted Rights Legend 1-3

S

Safety Information 1-6

Safety Precautions

 For the Operator 1-6

 For the Service Engineer 2-14

Safety Symbols 1-7

SDH Frequency Offsets 3-64, 3-65

Self Test 3-5

Serial Number Plate 1-4

Shipping Container Inspection 2-1

SPDH Receiver Monitor Levels 3-39, 3-78

Statement of Compliance 1-10

STM-1 Transmitter Output Waveshape 3-66, 3-70

STM-1/STM-4 Optical Interface 3-82

Index

Storage and Shipment 1-4

Symbols, Safety 1-7

T

TRANSMIT 2,8,34,140 OUT 2-6

V

VGA Connector 2-11

W

Warning Symbols 2-10

Warranty 1-1

Weight and Dimensions 1-5

Hewlett-Packard Sales and Service Offices

The following information was correct at the time of printing. If you have difficulty contacting an HP office, an up-to-date list of contacts is available through the HP Website at URL <http://www.tmo.hp.com/tmo/index.html>.

Australia/New Zealand

Australia:

Hewlett-Packard Australia Ltd.
31-41 Joseph Street
PO Box 221
Blackburn, Victoria 3130
Phone Number: 1-800-629-485
Fax: (61-3) 9272-0749

China:

China Hewlett-Packard Co. Ltd.
HP Building
No. 2, dong San Huan Nan Lu
Chao Yang District
Beijing 100022, PRC
Phone Number: (86-10) 6564-3888, 800-810-0189
Fax: (86-10) 6566-8250

India:

Hewlett-Packard India
Telesales Engineer
Test & Measurement
Chandiwala Estate, Kalkaji
New Delhi -110019
E-mail HPI Test & Measurement Telesales
Phone Number: (91/11)6906156 /6826262
or 6826000 ext. 6156
Fax: (91/11)6826027

Korea, Republic of:

Hewlett-Packard Korea Ltd.
25-12, Yoido-dong
Youngdeungpo-ku

Seoul, 150-010

Phone Number: (82-2) 769-0800

Fax: (82-2) 786-1083

Malaysia:

Hewlett-Packard Sales (M) Sdn Bhd
HP DIRECT Test and Measurement
Ground Floor, Wisma Cyclecarri
288, Jalan Raja Laut
50350 Kuala Lumpur
Malaysia
Phone Number: 1-800-88-8848
(6-03) 291-0213
Fax: (6-03) 298-9157
E-Mail Address: hp-direct_my@hp.com

New Zealand:

Hewlett-Packard (New Zealand) Ltd.
186-190 Willis Street
PO Box 9443
Wellington
Phone Number: 0800-738-378
Fax: 64-4-802-6881

Singapore:

Hewlett-Packard Singapore (Sales) Pte Ltd.
450 Alexandra Road
Singapore 119960
Phone Number: 1800 3758100
Fax: (65) 275-9841
E-Mail Address: hpdirect_sgp@hp.com

Hewlett-Packard Sales and Service Offices (continued)

Taiwan:

Hewlett-Packard Taiwan Ltd.
Hewlett-Packard Building
8/F No. 337 Fu-Hsing North Road
Taipei, 105
Phone Number: 080-212-535
Fax: (886-2) 2718-9860
HP DIRECT Basic Tools toll free: 0800-47866,

Thailand:

Hewlett-Packard (Thailand) Ltd.
23rd-25th floor Vibulthani Tower 2
3199 Rama IV Road
Klong Toey, Bangkok 10110
Phone Number: 661-3999, (088) 225-802

Europe

Austria:

Hewlett-Packard GmbH
HP DIRECT Österreich
Herrenberger Str. 110-140
D-71034 Böblingen
Deutschland
aus Österreich
Phone Number: (01) 25000-7171
Fax: (01) 25000-7172
E-Mail Address: Messtechnik_vertrieb@hp.com

Belgium:

Hewlett-Packard Belgium SA/NV
Test & Measurement
Boulevard de la Woluwe 100-102
B-1200 Brussels
Phone Number: (32/2) 778 3417
Fax: (32/2) 778 3414

Czech Republic:

T&M DIRECT, s.r.o.
Technická 2
166 27 Praha 6
Phone Number: 420/2/2435 5808
Fax: 420/2/2435 5809

Denmark:

Hewlett-Packard A/S
T&M Direct
Kongevejen 25
3460 Birkerød
Phone Number: 45 99-15-15
Fax: 45 82-06-30
E-Mail Address: test_measurement@hp.dk

Finland:

Hewlett-Packard Oy
Piispankalliontie 17
02200 ESPOO
Finland
P.O. Box Address:
P.O. Box 68
02201 ESPOO
Finland
Phone Number: 358-9-8872 2100
Fax: 358-9-8872 2923
E-Mail Address: tmodirect@finland.hp.com

Hewlett-Packard Sales and Service Offices (continued)

France:

Hewlett-Packard France
HP DIRECT
Test et Mesure
Z.A. de Courtaboeuf
1, Avenue du Canada
91947 Les Ulis Cedex
Phone Number: 01 69 29 41 14
Fax: 01 69 82 65 09

Germany:

Hewlett-Packard GmbH
HP DIRECT
Herrenberger Str. 140
71034 Böblingen
Phone Number: (0180) 524-63 33
Fax: (0180) 524-63 36
E-Mail Address: Messtechnik_vertrieb@hp.com

Greece:

HP DIRECT
G-SYSTEMS
76, Ymittou Street
11634 Athens
Phone Number: 01 726 40 26
Fax: 01 726 40 20

Ireland:

Hewlett-Packard Ireland Ltd.
HP DIRECT
Hewlett-Packard House
Stradbroke Road
Blackrock Co.
Dublin
Phone Number: 01 615 8222
Fax: 01 284 5134

Italy:

Hewlett-Packard Italiana S.p.A.
HP DIRECT
Soluzioni di Misura e Collaudo
Via G. Di Vittorio, 9
20063 Cernusco s/N (MI)
Phone Number: 39 02 9212 2241
Fax: 39 02 9210 4069
E-Mail Address:
hpi_direct@hp-italy-gen3.om.hp.com

Netherlands:

Hewlett-Packard Nederland B.V.
HP T&M DIRECT
Startbaan 16
1187 XR Amstelveen
Phone Number: 020-547 6669
Fax: 020-547 7765
E-Mail Address:
tmdept_hpnl@hp-netherlands-gen1.om.hp.com

Norway:

Hewlett-Packard Norge A/S
T&M Direkte Drammensveien 169
Postboks 60 Skoeyen 0212 OSLO
Norway
Phone Number: +47 2273 5759
Fax: +47 2273 5619
E-Mail Address: test_measurement@norway.hp.com

Poland:

Malkom
Ul. Bodycha 18
02-495 Warszawa
Phone Number: 48-22-7230066
Contact: Beata Sniecikowska

Hewlett-Packard Sales and Service Offices (continued)

Spain:

Hewlett-Packard Española, S.A.
HP DIRECT
Ctra. N-VI, KM 16,500
28230 Las Rozas, Madrid
Phone Number: 34 91 631.13.23
Fax: 34 91 631.14.69

Sweden:

Hewlett-Packard Sverige AB
HP Test & Mät-systems kundcenter
Skalholtskatan 9
S-164 97 KISTA
Sweden
Phone Number: (08) 444 2277
Fax: (08) 444 2525
E-Mail Address:
test-measurement@sweden.hp.com

Switzerland:

Hewlett-Packard (Schweiz) AG
HP DIRECT Schweiz
Elektronische Meßtechnik
In der Luberzen 29
8902 Urdorf/Zürich
German speaking:
Phone Number: (01) 735 72 00
Fax: (01) 735 72 90
French speaking:
Tel: (022) 780 4361
Fax: (022) 780 4180
E-Mail Address: Messtechnik_vertrieb@hp.com

United Kingdom:

Hewlett-Packard Ltd.
Test & Measurement
Cain Road

Bracknell, Berkshire
RG12 1HN
Phone Number: 01344-366666
Fax: 01344-362852
E-Mail Address: uktmo_sales@hp.com

Japan:

Hewlett-Packard Japan Ltd.
Measurement Assistance Center
9-1, Takakura-Cho, Hachioji-Shi
Tokyo, 192-8510
Phone Number: 81-426-56-7832
Additional phone number(s): 0120-421-345
Fax: 81-426-56-7843
Additional Fax: 0120-421-678

Latin America

Brazil:

Hewlett-Packard Brasil S.A.
Depto. Teste e Medicao
Alameda Rio Negro, 750
06454-000-Alphaville-Barueri
Sao Paulo, Brazil
Phone Number: (55-11) 7297-8600
Fax: (55-11) 7297-8171

Mexico:

Hewlett-Packard de Mexico, S.A. de C.V.
Prolongacion Reforma No. 700
Col. Lomas de Santa Fe
01210 Mexico D.F.
Phone Number: (52-5) 258-4392
Fax: (52-5) 258-4301
HP DIRECT: 01 800 50648

Hewlett-Packard Sales and Service Offices (continued)

Middle East and Africa

Israel:

HP DIRECT

C.M.S. LTD.

11, Hashelosh St.

Tel-Aviv 67060

Phone Number: 03 53 80 377

Fax: 03 53 76 505

Hewlett-Packard

HP DIRECT

11, Hashlosha St.

Tel-Aviv 67060

Phone Number: 03 53 80 377

Fax: 03 53 76 505

South Africa:

Hewlett-Packard South Africa (Pty.) Ltd.

HP DIRECT

Private Bag

WENDYWOOD 2148

Phone Number: 27-11-806 1173

Fax: 27-11-806 1213

North America

Canada:

Hewlett-Packard (Canada) Ltd.

HP DIRECT

5150 Spectrum Way

Mississauga, ON

L4W 5G1

Phone Number: 1-877-894-4414

Fax: 1-(905) 206-4700

Hewlett-Packard (Canada) Ltd.

Test & Measurement Business Centre

2670 Queensview Drive

Ottawa, Ontario K2B 8K1

Phone Number: 1-800-276-8661

Fax: 1-800-746-4866

United States:

For Technical Product Information:

Hewlett-Packard Co.

Test & Measurement Call Center

9780 S. Meridian Blvd.

Englewood, CO 80112

Phone Number: (800) 452-4844

Fax: (303) 662-3726

For Quotation/Order Information:

Hewlett-Packard Co.

Test & Measurement Business Center

9780 S. Meridian Blvd.

Englewood, CO 80112

Phone Number: (800) 829-4444

Fax: (800) 829-4433

For Federal Government Orders:

Hewlett-Packard Co.

P.O.Box 1487

Rockville, MD 20849-1487

Phone Number: (800) 468-8347

Fax: (800) 437-1085

California

Hewlett-Packard Co. (2451)

301 E. Evelyn Avenue

Mountain View, CA 94041

Phone Number: (800) 403-0801

Fax: (888) 857-8161

Hewlett-Packard Co. (24BR)

10090 Foothill Blvd.

Hewlett-Packard Sales and Service Offices (continued)

Roseville, CA 95747-7102

Phone Number: (800) 403-0801

Fax: (888) 857-8161

Colorado

Hewlett-Packard Co. (2452)

24 Inverness Place East

Englewood, CO 80112

Phone Number: (800) 403-0801

Fax:(888) 857-8161

New Jersey

Hewlett-Packard Co. (4401)

150 Green Pond Road

Rockaway, NJ 07866

Phone Number: (800) 403-0801

Fax: (888) 857-8161

Texas

Hewlett-Packard Co. (3185)

930 E. Campbell Road

Richardson, TX 75081

Phone Number: (800) 403-0801

Fax: (888) 857-8161