

Agilent 81250 Parallel Bit Error Ratio Tester

**System Programming
Guide and
SCPI Reference**



Agilent Technologies

Important Notice

© Agilent Technologies, Inc. 2003

Manual Part Number

5988-4886EN

Revision

Revision 5.5, December 2003

Printed in Germany

Agilent Technologies
Herrenberger Straße 130
D-71034 Böblingen
Germany

Authors: t3 medien GmbH

Warranty

The material contained in this document is provided "as is," and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as "Commercial computer software" as defined in DFAR 252.227-7014 (June 1995), or as a "commercial item" as defined in FAR 2.101(a) or as "Restricted computer software" as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies' standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notices

CAUTION

A CAUTION notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING

A WARNING notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

Trademarks

Windows NT® and MS Windows® are U.S. registered trademarks of Microsoft Corporation.

Contents

Programming Interfaces	19
<hr/>	
Programming Models	20
Agilent 81250 String Interface Library	22
Error Handling	23
Connect_HP81200	23
Call_HP81200	24
GetErrStr_HP81200	25
Disconnect_HP81200	25
Example Implementations	26
Command Line Interface	28
Overview of the SCPI Command Structure	29
<hr/>	
Command Syntax	30
Hierarchical Structure	30
Conventions Used in the Command Reference	30
Instrument Commands and Queries Syntax	31
Linking Commands	31
The Command Tree	32
DVT Subsystem and Virtual Instruments	33
Multiple Parameter Access	34
Example Programs	37
Typical SCPI Programming Sequence	38
Example C++ Program	40
SCPI Commands Overview	43
Generic Administration Commands	44
Virtual Instruments Administration Commands	44
Mass Memory Commands	45
Segment Editing Commands	46
Global Commands	48
Clock Reference Input Commands	49
External Input Commands	50
Trigger Output Commands	50
Port Administration Commands	51

Terminal Administration Commands	52
Connector Administration Commands	52
Clockgroup Administration Commands	53
Sequence Commands	53
Synchronization Commands	54
Analyzer Commands	55
Level Parameter Commands	55
Amplitude/Offset Correction Factor Commands	56
Timing Parameter Commands	57
MUX Parameter Commands	58
DeMUX Parameter Commands	59
DeMUX Rewiring Commands	59
Delay Control Parameter Commands	60
Input Parameter Commands	60
Optical Input Commands	62
Output Parameter Commands	63
Optical Output Commands	64
Clock Trigger Output Commands	65
Auxiliary Out Commands	65
Performance Parameter Commands	66
Format Parameter Commands	66
Commands in the DVT Subsystem	67
<hr/>	
Example: Use of :DVT Subsystem Commands	68
Top-Level Commands	69
:DVT:IDN?	69
:SYSTem Subsystem	70
:DVT:SYSTem:ERRor?	70
:INSTrument Subsystem	71
:DVT:INSTrument:LIST?	71
:DVT:INSTrument:RESource:LIST?	71
:INSTrument:HANDle Subsystem	72
:DVT:INSTrument:HANDle:CREate?	72
:DVT:INSTrument:HANDle:LIST?	73
:DVT:INSTrument:HANDle:DESTroy	73

:MMEMory Subsystem	74
:DVT:MMEMory:SETTing:EXPort?	74
:DVT:MMEMory:SETTing:IMPort	75
Commands in DSR Application Subsystems	77
<hr/>	
Administration Commands	78
:<Handle>:IDN?	78
:<Handle>:OPC?	78
:SYSTem Subsystem	79
:<Handle>:SYSTem:ERRor?	79
:<Handle>:SYSTem:CINformation?	80
:<Handle>:SYSTem:TEST:MODule	81
:<Handle>:SYSTem:TEST:GLOBal	82
:<Handle>:MODule:SREVisions	82
:<Handle>:SYSTem:MQUeue[:READ]?	83
:<Handle>:SYSTem:MQUeue:LENGth?	83
:<Handle>:SYSTem:PON[:STATus]	83
:SYSTem:CLient Subsystem	84
:<Handle>:SYSTem:CLient[:HANDle]?	84
:<Handle>:SYSTem:CLient:LOCK	84
:<Handle>:SYSTem:CLient:BLOCK	85
:<Handle>:SYSTem:CLient:UNLock	85
:CONFIguration Subsystem	86
:<Handle>:CONFIguration:CGRoups(*)?	86
:<Handle>:CONFIguration:CGRoups(*):MODules(*)?	86
:<Handle>:CONFIguration:CGRoups(*):MODules(*): CONNectors(*)?	87
:<Handle>:CONFIguration:CGRoups(*):MODules(*): CONNectors(*):TYPE?	87
:<Handle>:CONFIguration:STYPes?	87
:<Handle>:CONFIguration:PROFile[:VALue]	88
:<Handle>:CONFIguration:PROFile[:VALue]?	88
:<Handle>:CONFIguration:PROFile:REMOve	88
:<Handle>:CONFIguration:PROFile:LIST?	89
:MMEMory Subsystem	90
:<Handle>:MMEMory:LIST?	90
:<Handle>:MMEMory:INformation?	91
:<Handle>:MMEMory:SEGMent:LOAD	92

:<Handle>:MMEMory:SEGMENT:SAVE	93
:<Handle>:MMEMory:SEGMENT:GET?	94
:<Handle>:MMEMory:SETTING:NAME?	94
:<Handle>:MMEMory:SETTING:LOAD	95
:<Handle>:MMEMory:SETTING:SAVE	95
:<Handle>:MMEMory:SETTING:NEW	96
:<Handle>:MMEMory:SETTING:DELETE	96
:EDIT:SEGMENT(*) Subsystem	97
:<Handle>:EDIT:SEGMENT:OPEN?	98
:<Handle>:EDIT:SEGMENT(*):SAVE	99
:<Handle>:EDIT:SEGMENT(*):DELETE	100
:<Handle>:EDIT:SEGMENT(*):CREATE?	100
:<Handle>:EDIT:SEGMENT(*):EXISTS?	101
:<Handle>:EDIT:SEGMENT(*):RPATH?	102
:<Handle>:EDIT:SEGMENT(*):CLOSE	103
:<Handle>:EDIT:SEGMENT(*):PATTERN:DATA	103
:<Handle>:EDIT:SEGMENT(*):PATTERN:DATA?	104
:<Handle>:EDIT:SEGMENT(*):PATTERN:CODING	106
:<Handle>:EDIT:SEGMENT(*):PATTERN:CODING?	107
:<Handle>:EDIT:SEGMENT(*):PATTERN:ERROR:FIRST?	107
:<Handle>:EDIT:SEGMENT(*):PATTERN:ERROR:NEXT?	108
:<Handle>:EDIT:SEGMENT(*):PATTERN:ERROR:PREVIOUS?	108
:<Handle>:EDIT:SEGMENT(*):PATTERN:FIND:FIRST?	109
:<Handle>:EDIT:SEGMENT(*):PATTERN:FIND:NEXT?	111
:<Handle>:EDIT:SEGMENT(*):PATTERN:FIND:PREVIOUS?	111
:<Handle>:EDIT:SEGMENT(*):PATTERN:LENGTH?	112
:<Handle>:EDIT:SEGMENT(*):PATTERN:WIDTH?	112
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:COPY	113
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:PASTE	113
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:FILL	114
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:INVERT	115
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:MIRROR	116
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:INSERT	117
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:DELETE	117
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:CONVERSE	118
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:SERIALIZE	119
:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:DESERIALIZE	120
:<Handle>:EDIT:SEGMENT(*):PARAMETER:LENGTH?	120
:<Handle>:EDIT:SEGMENT(*):PARAMETER:LIST?	121

:<Handle>:EDIT:SEGMENT(*):PARAMeter[:VALue]?	121
:<Handle>:EDIT:SEGMENT(*):PARAMeter[:VALue]	122
:<Handle>:EDIT:SEGMENT(*):PARAMeter:REMOve	122
:<Handle>:EDIT:SEGMENT(*):TYPE	122
:<Handle>:EDIT:SEGMENT(*):TYPE?	123
[:CGROUP(*)] Subsystem	123
:<Handle>[:CGROUP(*)]:CINFORMATION?	124
[:CGROUP(*)]:MCLock Subsystem	125
:<Handle>[:CGROUP(*)]:MCLock:SOURce[:VALue]	125
:<Handle>[:CGROUP(*)]:MCLock:SOURce[:VALue]?	125
[:CGROUP(*)]:MODULE(*) Subsystem	126
:<Handle>[:CGROUP(*)]:MODULE(*):CINFORMATION?	126
:<Handle>[:CGROUP(*)]:MODULE(*):TYPE?	127
:<Handle>[:CGROUP(*)]:MODULE(*):SLOT?	127
:<Handle>[:CGROUP(*)]:MODULE(*):FRAME?	127
:<Handle>[:CGROUP(*)]:MODULE(*):NAME?	127
:<Handle>[:CGROUP(*)]:MODULE(*):CNAMES?	128
[:CGROUP(*)]:MODULE(*):CONNECTOR(*) Subsystem	129
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*): CINFORMATION?	129
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):TYPE?	130
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):NAME?	130
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):TNAME?	130
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):CALIBRATION: CDELAY	131
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):CALIBRATION: CDELAY?	131
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):CALIBRATION: ZDELAY	131
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):CALIBRATION: ZDELAY?	132
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):SPECIES[: VALue]?	132
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):SPECIES: STATE	132
:<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):SPECIES: STATE?	133

[:CGRoup(*)][:SOURce]:TRIGger Subsystem	134
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:DELay	134
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:DELay?	134
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:MUX	135
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:MUX?	135
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:OUTPut[:STATe]	135
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:OUTPut[:STATe]?	136
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:HIGH	136
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:HIGH?	136
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:LOW	137
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:LOW?	137
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:TVOLTage	137
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:TVOLTage?	138
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:IMPedance:EXTernal	138
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:IMPedance:EXTernal?	138
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:MODE	139
:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:MODE?	139
:SGENeral Subsystem	140
:SGENeral:INFormation Subsystem	141
:<Handle>:SGENeral:INFormation:PClasses?	141
:SGENeral:GLOBal Subsystem	142
:<Handle>:SGENeral:GLOBal:CONNect	142
:<Handle>:SGENeral:GLOBal:CONNect?	142
:<Handle>:SGENeral:GLOBal:CALibration:PUSe PASSive	143
:<Handle>:SGENeral:GLOBal:CALibration:SELF DELay	143
:<Handle>:SGENeral:GLOBal:DOFFset	143
:<Handle>:SGENeral:GLOBal:DOFFset?	144
:<Handle>:SGENeral:GLOBal:FETCh:ERRor:ANY?	144
:<Handle>:SGENeral:GLOBal:PERiod	144
:<Handle>:SGENeral:GLOBal:PERiod?	145
:<Handle>:SGENeral:GLOBal:FREQuency	145
:<Handle>:SGENeral:GLOBal:FREQuency?	145
:<Handle>:SGENeral:GLOBal:MUX?	146

:<Handle>:SGENeral:GLOBal:MUX	146
:<Handle>:SGENeral:GLOBal:PLL:DState?	149
:<Handle>:SGENeral:GLOBal:PLL:State?	150
:SGENeral:GLOBal:CONFigure Subsystem	151
:<Handle>:SGENeral:GLOBal:CONFigure?	151
:<Handle>:SGENeral:GLOBal:CONFigure:CAPture	151
:<Handle>:SGENeral:GLOBal:CONFigure[:ECOut]	152
:<Handle>:SGENeral:GLOBal:CONFigure:ECAPture	152
:<Handle>:SGENeral:GLOBal:CONFigure:CCAPture	153
:SGENeral:GLOBal:INITiate:CONTInuous Subsystem	154
:<Handle>:SGENeral:GLOBal:INITiate:CONTInuous	154
:<Handle>:SGENeral:GLOBal:INITiate:CONTInuous?	154
:SGENeral:GLOBal:SYStem Subsystem	155
:<Handle>:SGENeral:GLOBal:SYStem:State?	155
:SGENeral:GLOBal:SEQuence Subsystem	156
:<Handle>:SGENeral:GLOBal:SEQuence[:VALue]	157
:<Handle>:SGENeral:GLOBal:SEQuence[:VALue]?	161
:<Handle>:SGENeral:GLOBal:SEQuence:EVENTs	162
:<Handle>:SGENeral:GLOBal:SEQuence:EVENTs?	164
:<Handle>:SGENeral:GLOBal:SEQuence:FORCe	165
:<Handle>:SGENeral:GLOBal:SEQuence:LLEVel?	165
:<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol	166
:<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol?	166
:<Handle>:SGENeral:GLOBal:SEQuence:State?	166
:SGENeral:GLOBal:SYNChronization Subsystem	167
:<Handle>:SGENeral:GLOBal:SYNChronization:USED?	168
:<Handle>:SGENeral:GLOBal:SYNChronization:BERThreshold	168
:<Handle>:SGENeral:GLOBal:SYNChronization:BERThreshold?	169
:<Handle>:SGENeral:GLOBal:SYNChronization:SMODE	169
:<Handle>:SGENeral:GLOBal:SYNChronization:SMODE?	170
:<Handle>:SGENeral:GLOBal:SYNChronization:APSelect	170
:<Handle>:SGENeral:GLOBal:SYNChronization:APSelect?	171
:<Handle>:SGENeral:GLOBal:SYNChronization:APAligment	171
:<Handle>:SGENeral:GLOBal:SYNChronization:APAligment?	172
:<Handle>:SGENeral:GLOBal:SYNChronization:PACCuracy	172

:<Handle>:SGENERal:GLOBal:SYNChronization:PACCuracy?	172
:SGENERal:GLOBal:TRIGger Subsystem	173
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]	173
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]?	174
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDRList?	174
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDR	174
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDR?	175
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK[:VALue]?	175
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MEASurement[:DIRect]	175
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MULTIplier	176
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MULTIplier?	176
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:DIVider	176
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:DIVider?	177
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:RCLock:DETect	177
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:CLock:MEASurement	177
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:TVOLtage	178
:<Handle>:SGENERal:GLOBal:TRIGger[:SEQuence][:LAYer]:TVOLtage?	178
:SGENERal:GLOBal:ARM Subsystem	179
:<Handle>:SGENERal:GLOBal:ARM[:SEQuence][:LAYer][:SOURce]	180
:<Handle>:SGENERal:GLOBal:ARM?	181
:<Handle>:SGENERal:GLOBal:ARM[:SEQuence][:LAYer]:SENSe	181
:<Handle>:SGENERal:GLOBal:ARM[:SEQuence][:LAYer]:SENSe?	181

:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]: THReshold	182
:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]: THReshold?	182
:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]: TVOLtage	182
:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]: TVOLtage?	183
Timing Parameter Commands	184
:PULSe:DELay	185
:PULSe:DELay?	186
:PULSe:DELay:CYCLes	186
:PULSe:DELay:CYCLes?	187
:PULSe:DELay:TIME	188
:PULSe:DELay:TIME?	188
:PULSe:CROSSing	189
:PULSe:CROSSing?	190
:PULSe:WIDTh	191
:PULSe:WIDTh?	191
:PULSe:DCYCLe	192
:PULSe:DCYCLe?	192
:PULSe:HOLD	193
:PULSe:HOLD?	193
:PULSe:TRANsition[:LEADing]	194
:PULSe:TRANsition[:LEADing]?	195
:PULSe:TRANsition:TRAILing	195
:PULSe:TRANsition:TRAILing?	196
:PULSe:TRANsition:CAConfiguration[:LEADing]	197
:PULSe:TRANsition:CAConfiguration[:LEADing]?	198
:PULSe:TRANsition:CAConfiguration:TRAILing	199
:PULSe:TRANsition:CAConfiguration:TRAILing?	200
:MUX	201
:MUX?	201
Parameter Commands for MUX and DEMUX Modules	202
:VOLTage:AMPLitude	206
:VOLTage:AMPLitude?	206
:VOLTage:OFFSet	207
:VOLTage:OFFSet?	207
:VOLTage:OFFSet:ENABle	208

:VOLTage:OFFSet:ENABle?	208
:OUTPut:EATTenuator	209
:OUTPut:EATTenuator?	209
:OUTPut:DELay:SWEep	210
:OUTPut:DELay:SWEep?	211
:OUTPut:DELay:SWEep:MODE	211
:OUTPut:DELay:SWEep:MODE?	212
:OUTPut:DELay:SWEep:PROM	213
:INPut:OCOMpensation	214
:INPut:OCOMpensation?	214
:TRIGger	215
:TRIGger?	215
:TRIGger:MODE	216
:TRIGger:MODE?	216
DeMUX Rewiring Parameter Commands	217
<Handle>:SGENeral:GLOBal:SYNChronization:REWire	219
<Handle>:SGENeral:GLOBal:SYNChronization:REWire?	219
<Handle>:SGENeral:GLOBal:SYNChronization:RMODE	220
<Handle>:SGENeral:GLOBal:SYNChronization:RMODE?	221
<Handle>:SGENeral:GLOBal:SYNChronization:RCH	221
<Handle>:SGENeral:GLOBal:SYNChronization:RCH?	222
<Handle>:SGENeral:PDATa:DMUX:STAGe	222
<Handle>:SGENeral:PDATa:DMUX:STAGe?	223
<Handle>:SGENeral:PDATa:DMUX:STAGe:OUT	223
<Handle>:SGENeral:PDATa:DMUX:STAGe:OUT?	224
Level Parameter Commands	225
:VOLTage[:LEVel][:IMMEDIATE]:HIGH	225
:VOLTage[:LEVel][:IMMEDIATE]:HIGH?	226
:VOLTage[:LEVel][:IMMEDIATE]:LOW	227
:VOLTage[:LEVel][:IMMEDIATE]:LOW?	228
:VOLTage[:LEVel][:IMMEDIATE]:CAConfiguration:LOW	229
:VOLTage[:LEVel][:IMMEDIATE]:CAConfiguration:LOW?	230
:VOLTage[:LEVel][:IMMEDIATE]:SEMode	231
:VOLTage[:LEVel][:IMMEDIATE]:SEMode?	232
:VOLTage[:LEVel][:IMMEDIATE]:SEMode:AVAIlable?	232
:SENSe:VOLTage:RANGe	233
:SENSe:VOLTage:RANGe?	233

Amplitude/Offset Correction Factor Commands	234
:CALibration[:VOLTage]:OCFactor	235
:CALibration[:VOLTage]:OCFactor?	235
:CALibration[:VOLTage]:ACFactor	236
:CALibration[:VOLTage]:ACFactor?	236
:CALibration[:VOLTage]:HOLD	237
:CALibration[:VOLTage]:HOLD?	237
Delay Control Parameter Commands	239
:DCONtrol[:DEViation]?	239
:DCONtrol:SENSitivity	240
:DCONtrol:SENSitivity?	240
:DCONtrol:SOURce	241
:DCONtrol:SOURce?	242
:DCONtrol:STATe	243
:DCONtrol:STATe?	244
Input Parameter Commands	245
:INPut[:STATe]	245
:INPut[:STATe]?	245
:INPut:POLarity	246
:INPut:POLarity?	246
:INPut:TYPE	247
:INPut:TYPE?	248
:INPut:MODE	248
:INPut:MODE?	249
:INPut:TVOLTage	250
:INPut:TVOLTage?	250
:INPut:THReshold	251
:INPut:THReshold?	251
:INPut:IMPedance[:INTernal]	252
:INPut:IMPedance[:INTernal]?	252
:INPut:SEQuence:[LAYer:SOURce:]CLOCK	252
:INPut:SEQuence:[LAYer:SOURce:]CLOCK?	253
:INPut:SERial	254
:INPut:SERial?	254
:INPut:DELay	255
:INPut:DELay?	255
:INPut:DELay:CYCLes	256
:INPut:DELay:CYCLes?	256

:INPut:DELay:TIME	257
:INPut:DELay:TIME?	257
:INPut:DELay:ACTual?	258
:INPut:DELay:SWEEp	259
:INPut:DELay:SWEEp?	259
:INPut:TCONfig	260
:INPut:TCONfig?	261
:INPut:DIMPedance	261
:INPut:DIMPedance?	262
:INPut:DISConnect:MODE?	262
:INPut:DISConnect:MODE	263
Optical Input Commands	263
:INPut:OPTic[:STATe][:VALue]	264
:INPut:OPTic[:STATe][:VALue]?	264
:INPut:OPTic:POWer:UNIT[:VALue]	265
:INPut:OPTic:POWer:UNIT[:VALue]?	265
:INPut:OPTic:POWer:THReshold[:VALue]	266
:INPut:OPTic:POWer:THReshold[:VALue]?	266
:INPut:OPTic:WAVelength[:VALue]	266
:INPut:OPTic:WAVelength[:VALue]?	267
:INPut:OPTic:MEASure	267
:INPut:OPTic:DLCalibration	267
Output Parameter Commands	268
:OUTPut[:STATe]	268
:OUTPut[:STATe]?	269
:OUTPut:POLarity	270
:OUTPut:POLarity?	270
:OUTPut:CSTate	271
:OUTPut:CSTate?	271
:OUTPut:TVOLtage	272
:OUTPut:TVOLtage?	272
:OUTPut:IMPedance:EXTErnal	273
:OUTPut:IMPedance:EXTErnal?	273
:OUTPut:TCONfig	274
:OUTPut:TCONfig?	275
:OUTPut:DIMPedance:EXTErnal	276
:OUTPut:DIMPedance:EXTErnal?	276
:OUTPut:CAConfiguration[:MODE]	277

:OUTPut:CAConfiguration[:MODE]?	278
:OUTPut:DISConnect:MODE?	278
:OUTPut:DISConnect:MODE	279
Optical Output Commands	280
:OUTPut:OPTic[:STATe][:VALue]	281
:OUTPut:OPTic[:STATe][:VALue]?	282
:OUTPut:OPTic:METHod[:VALue]	283
:OUTPut:OPTic:METHod[:VALue]?	283
:OUTPut:OPTic:POWer:UNIT[:VALue]	284
:OUTPut:OPTic:POWer:UNIT[:VALue]?	284
:OUTPut:OPTic:POWer:AVERAge[:VALue]	285
:OUTPut:OPTic:POWer:AVERAge[:VALue]?	285
:OUTPut:OPTic:POWer:MAMPlitude[:VALue]	286
:OUTPut:OPTic:POWer:MAMPlitude[:VALue]?	287
:OUTPut:OPTic:POWer:HIGH[:VALue]	287
:OUTPut:OPTic:POWer:HIGH[:VALue]?	288
:OUTPut:OPTic:POWer:LOW[:VALue]	288
:OUTPut:OPTic:POWer:LOW[:VALue]?	289
:OUTPut:OPTic:ERATio[:VALue]	289
:OUTPut:OPTic:ERATio[:VALue]?	290
:OUTPut:OPTic:ERATio:UNIT[:VALue]	290
:OUTPut:OPTic:ERATio:UNIT[:VALue]?	291
Clock Output Commands	292
:CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:HIGH	292
:CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:HIGH?	292
:CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:LOW	293
:CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:LOW?	293
:CLOCK[:SOURce]:PULSe:DELay:SWEEp	293
:CLOCK[:SOURce]:PULSe:DELay:SWEEp?	294
:CLOCK:OUTPut:IMPedance:EXTErnal	294
:CLOCK:OUTPut:IMPedance:EXTErnal?	294
:CLOCK:OUTPut:DIMPedance:EXTErnal	295
:CLOCK:OUTPut:DIMPedance:EXTErnal?	295
:CLOCK:OUTPut:TCONfig	296
:CLOCK:OUTPut:TCONfig?	297
:CLOCK:OUTPut:TVOLTage	297
:CLOCK:OUTPut:TVOLTage?	298

Auxiliary Out Commands	298
:AOUT[:MONitor]	298
:AOUT[:MONitor]?	299
Port Administration Commands	300
:APPend	300
:LIST?	301
:ATYPes?	301
:DElete	301
:REName	302
:NAME?	302
:NUMBer?	302
:TYPE?	303
:CALibration:CDELay	303
:CALibration:CDELay?	303
:SPECies?	304
Terminal Administration Commands	305
:APPend	305
:LIST?	305
:DElete	306
:FETCh:SSTatus?	306
:REName	306
:NAME?	307
:TYPE?	307
:MOVE	307
:CALibration:CDELay	308
:CALibration:CDELay?	308
Connector Administration Commands	309
:REMove	309
:TERMinal(*):[TO]	310
:TERMinal(*):[TO]?	311
Error Analysis Commands	312
:FETCh:ERRor:ANY?	312
:FETCh[:ECOunt]?	312
:ECOunt:RESet	315
Clock Mode Commands	316
:SIGNal:MODE	316
:SIGNal:MODE?	317

Format Parameter Commands	318
:FORMat	318
:FORMat?	319
Segment Import and Export Language	321
<hr/>	
The Language Syntax	322
Vector Variable Construct	322
Segment Construct	322
Name Construct	323
Options	323
StatePar Construct	324
StateSet Construct	324
Base Construct	324
Vector Width Construct	325
Vector Construct	325
Parameter Construct	326
Concepts	326
Coding	326
Scopes	328
Vector Padding and Clipping	330
Parameter Segments	331
Default Settings	333
Examples	333
Example: Memory Type Segment	334
Example: PRBS Type Segment	334
Example: PRWS Type Segment	335
Example: SFI5 Type Segment	335
Example Code	337
<hr/>	
Main.cpp Application Code Using VXI Plug&Play	338
Lib.cpp Interface Class Library Code	351
Main.cpp Application Code	356

Programming Interfaces

The Agilent 81250 provides, besides the user interface, the following control possibilities:

- VXI PnP

This is the recommended method for controlling the Agilent 81250. For details on using VXI PnP, see the `hp81200.hlp` provided in the help subdirectory of your Agilent 81250 installation.

- Agilent IO Libraries

You can use the Agilent IO Libraries for controlling the Agilent 81250 over a GPIB or emulated GPIB interface. For details, see the documentation delivered with the Agilent IO Libraries. The *LAN Programming Guide* (available in the online Help) also provides SICL- and VISA-based examples that can be used for non-LAN configurations.

- Agilent String Interface Library

The Agilent String Interface Library is a simple library available in C and VisualBasic for sending ASCII commands (such as SCPI commands) to and querying ASCII strings from the Agilent 81250. *“Agilent 81250 String Interface Library” on page 22* summarizes the major aspects to be considered when implementing programs for local control or for remote control via LAN using the string interface.

- Command Line Interface

In addition to these programming models, the Command Line Interface window provided by the user interface can be used to try out commands, and to store and replay simple sequences of commands (see *“Command Line Interface” on page 28*).


- Telnet and Socket Programs

The *LAN Programming Guide* (available in the online Help) provides the information necessary for controlling the Agilent 81250 using telnet or socket programming.

Programming Models

NOTE Instead of using the SCPI commands, we recommend to use the plug & play programming interface. For an online help on the VXIPNP functions, refer to `hp81200.hlp` provided in the help subdirectory of your Agilent 81250 installation.

The following picture shows the basic structure of the Agilent 81250's programming interfaces.

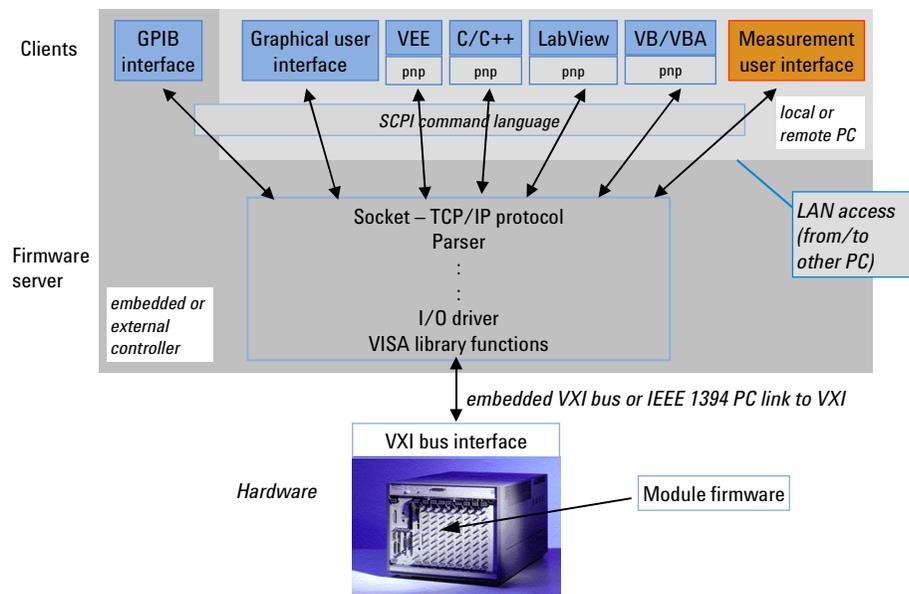

Firmware Server and SCPI Commands The user interface communicates with the firmware using the SCPI language. It implements a client-server architecture, allowing multiple clients to connect simultaneously.

The Agilent 81250 plug & play drivers also communicate with the firmware server using the SCPI language. Therefore, everything that can be done over the user interface can also be done using the other programming interfaces (with, of course, loss of comfort). For detailed information on the Agilent 81250 plug & play drivers, please refer to the corresponding online help files.

Tools and Programming Languages Depending on your configuration, tools like VEE or LabView, and the programming languages C/C++ and VisualBasic can be used for implementation.

NOTE You can also send SCPI commands directly to the system by using the Agilent String Interface Library. Examples and reference information are provided under “*Agilent 81250 String Interface Library*” on page 22.

Locking Mechanisms Different clients may operate on the same system concurrently using different interfaces. To avoid undesired interrupts, the Agilent 81250 features a locking mechanism, allowing each client to gain exclusive access to the system during critical operations.

The system can either be locked or blocked:

- With a locked system, commands from other clients are returned with an error message.
- With a blocked system, commands from other clients do not return until the system has been unlocked and the command has been executed.

Agilent 81250 String Interface Library

The Agilent 81250 String Interface library provides basic functions for connecting to an Agilent 81250 firmware server either on the local machine or via LAN.

C Implementation To implement the Agilent 81250 String Interface library in C, include the file `hp81200.h`.

VB Implementation To implement the Agilent 81250 String Interface library in VisualBasic, import the file `hp81200.bas` into your project.

The following commands are available:

C Command	VB Command	Described under:
Connect_HP81200	VB_CONNECT_HP81200	<i>“Connect_HP81200” on page 23</i>
Call_HP81200	VB_CALL_HP81200	<i>“Call_HP81200” on page 24</i>
GetErrStr_HP81200	VB_GETERRSTR_HP81200	<i>“GetErrStr_HP81200” on page 25</i>
Disconnect_HP81200	VB_DISCONNECT_HP81200	<i>“Disconnect_HP81200” on page 25</i>

A program using the Agilent 81250 String Interface library has the following structure:

- Connect to the firmware server.
- Send any SCPI commands or queries.
- Handle errors as necessary.
- Disconnect from the firmware server.

NOTE It is recommended that you explicitly disconnect from the firmware server at the end of your program. Otherwise, it may not be possible to connect again.

See *“Example Implementations” on page 26* for code examples in C and VisualBasic.

Error Handling

All functions in this library return an error code.

- A return value of 0 always means that the function call succeeded.
- A negative number indicates a server error. Use the function `GetErrStr_HP81200` with the error code as an argument to get a human-readable error string.
- A positive number indicates that the command execution failed. In this case, query the error queue corresponding to the last command. That means, if the last command started with `:dvt:`, send the command `:dvt:syst:err?` until the error queue is empty. If this does not locate the problem, send `<Handle>syst:err?` using the handle of your system.

Connect_HP81200

C Syntax `int HP81200_CDECL Connect_HP81200(const char *ServerName)`

VB Syntax `VB_CONNECT_HP81200(ByVal ServerName As String) As Long`

Description Connects to an Agilent 81250 server. This must be the first call when using the Agilent 81250 string interface library.

Parameters **ServerName** The machine name or IP address of the machine to which you want to connect. If left empty (NULL pointer or empty string), the local host is connected.

In general `ServerName` has the structure `[<host>[<sep><port>]]`

- `<host>` is the hostname in text (`mypc.bbn.hp`) or IP notation (`15.100.10.20`). The default is `127.0.0.1` (“localhost”).
- `<sep>` is a separator; this can be a null byte, space, comma, semicolon, colon, tab, or return. For clarity, a semicolon is used as separator in the examples.
- `<port>` is the port number as decimal string. The hard-coded default for port is `2203` or the contents of the environment variable `DVTDSRPORT`, if this is set.

Examples Examples of the server name are:

- `""`: all defaults, resolves to “`127.0.0.1; 2203`” (assuming environment variable `DVTDSRPORT` is not set)
- `"localhost"`: resolves to “`localhost; 2203`” (assuming environment variable `DVTDSRPORT` is not set)

- "; 7": override port, resolves to "127.0.0.1; 7"
- "15.100.10.20; 2208": fully specified host
- "mypc.bbn.hp.com; 2208": fully specified host

Call_HP81200

C Syntax `int HP81200_CDECL Call_HP81200(const char *Command,
char *Response,
int *BufferSize)`

VB Syntax `VB_CALL_HP81200(ByVal Command As String,
ByRef Response As String,
ByRef BufferSize As Long) As Long`

Description Sends a command to the Agilent 81250 server and gets the response.

Parameters **Command** Any valid SCPI command, as described in “*Overview of the SCPI Command Structure*” on page 29. If the command is a query, the response and size of the response are returned.

Response If the command is a query, the response is returned in this buffer.

BufferSize Size of the buffer allocated to receive the query result. On return, the variable holds the actual number of valid bytes in the buffer.

Return Value Returns 0 on success and a negative number for server problems (use “*GetErrStr_HP81200*” on page 25 to get an error message).

A positive number indicates that the command execution failed. Error messages can be read from the corresponding error queue (see “*Error Handling*” on page 23).

NOTE The parameter `Response` is a buffer area provided by the caller. The caller is responsible for reserving enough memory to hold the response.

To prevent buffer overruns, `BufferSize` defines the maximum number of bytes that can be written. This variable is set upon return to reflect the number of bytes actually written. If the response does not fit into the buffer, an error is returned.

GetErrStr_HP81200

C Syntax `int HP81200_CDECL GetErrStr_HP81200(int ErrCode,
char *ErrMsg, int *BufferSize)`

VB Syntax `VB_GETERRSTR_HP81200(ByVal ErrNum As Long,
ByRef ErrString As String,
ByRef BufferSize As Long) As Long`

Description Gets the error string if one of the calls returns a negative value (see “*Error Handling*” on page 23). This usually happens if the connection to the server or the creation of a handle fails.

Parameters **ErrCode** Error code returned by one of the other functions.

ErrMsg Buffer to receive a human-readable error string describing the error represented by ErrCode.

BufferSize Size of the buffer allocated to receive the error message (ErrMsg). On return, the variable holds the actual number of valid characters in the buffer.

NOTE The parameter Response is a buffer area provided by the caller. The caller is responsible for reserving enough memory to hold the response.

To prevent buffer overruns, BufferSize defines the maximum number of bytes that can be written. This variable is set upon return to reflect the number of bytes actually written. If the response does not fit into the buffer, an error is returned.

Disconnect_HP81200

C Syntax `int HP81200_CDECL Disconnect_HP81200()`

VB Syntax `VB_DISCONNECT_HP81200() As Long`

Description Disconnects from the Agilent 81250 server. This must be the last call when using the Agilent 81250 String Interface Library.

Example Implementations

The following examples show how these commands could be implemented in a C or VisualBasic environment.

C Example

The following code example connects to the firmware server on the defined machine at the defined port, queries the :DVT:IDN?, outputs the results, and disconnects.

```
#include <stdio.h>
#include <stdlib.h>
#include <string.h>

#include <hp81200.h>

#define BUFF_SIZE 1024

int main(int argc, char* argv[])
{
    int err = 0;
    char buffer[BUFF_SIZE];
    int bufSize= BUFF_SIZE;
    char* host;

    // Define host
    switch(argc)
    {
        case 1:
            host = "";
            break;
        case 2:
            host = argv[1];
        default:
            host = argv[1];
            strncat(host, "; ", 2);
            strncat(host, argv[2], strlen(argv[2]));
            break;
    }

    // Connect to host
    err = Connect_HP81200(host);
    if (err=0)
    {
        printf("Could not connect to host\n");
        return 0;
    }

    // Send :DVT:IDN?
    bufSize= BUFF_SIZE;
```

```

err = Call_HP81200(":DVT:IDN?", buffer, &bufSize);
if (err!=0)
    printf("Connected to: %s\n", buffer);
else
{
    // Get and output the error.
    bufSize= BUFF_SIZE;
    err = GetErrStr_HP81200(err, buffer, &bufSize);
    printf("Error generated: %s", buffer);
}

// Disconnect
err = Disconnect_HP81200();
return 0;
}

```

VisualBasic Example

NOTE To implement the example, you have to import the file hp81200.bas into your project.

The following code connects to the entered server, sends SCPI commands, and outputs the results.

```

Sub myHP81200()
' hp81200.bas has to be imported into your project
Dim err As Long
Dim buffer As String * 256
Dim bufSize As Long
Dim Cmd As String
Dim ServerName As String

' Request a server
ServerName = InputBox("Enter server name:", "Connect to Server")
err = VB_CONNECT_HP81200(ServerName)
' If the server is not available, output the error.
If err <> 0 Then
    buffer = ""
    bufSize = 256
    VB_GETERRSTR_HP81200 err, buffer, bufSize
    MsgBox "Could not connect due to error: " & vbCrLf & _
        buffer
    Exit Sub
End If

' Request and output commands
Do
    buffer = ""
    bufSize = 256
    Cmd = InputBox("Enter command:", "SCPI Command Input")

```


```

If Cmd = "" Then Exit Do
err = VB_CALL_HP81200(Cmd, buffer, bufSize)
' Output the results ...
If err = 0 Then
    MsgBox "Command " & Cmd & " succeeded." & vbCrLf & _
        vbCrLf & buffer
    ' ... or any errors
Else
    VB_GETERRSTR_HP81200 err, buffer, bufSize
    MsgBox "Command " & Cmd & " failed." & vbCrLf & _
        vbCrLf & buffer
End If
Loop
' Disconnect before closing
err = VB_DISCONNECT_HP81200
End Sub

```

Command Line Interface

The Agilent 81250 user interface features a Command Line window (*Command Line* in the *Go* menu) that allows you to enter SCPI commands and displays query results.

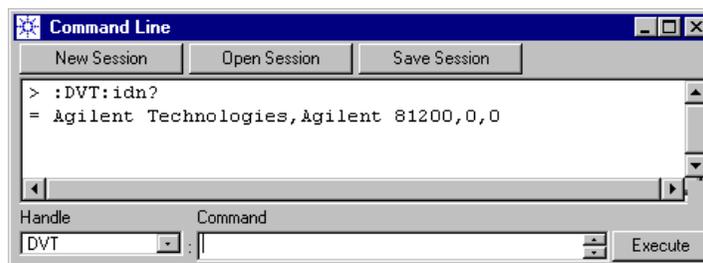

In this window, you can store and replay sequences of commands. This is very useful when implementing control programs, because you can test your SCPI commands and sequences before implementing them in your code.

Overview of the SCPI Command Structure

The device commands for the Agilent 81250 System follow the rules for SCPI Commands.

Some basic peculiarities of the command syntax used in this programming reference are described in *“Command Syntax” on page 30*.

The overall structure of the commands is described in *“The Command Tree” on page 32*.

A basic and a more advanced programming example using the Agilent 81250 SCPI commands are given in *“Example Programs” on page 37*.

“SCPI Commands Overview” on page 43 provides application-oriented access to the available SCPI commands. The individual commands are described in more detail in *“Commands in the DVT Subsystem” on page 67* and *“Commands in DSR Application Subsystems” on page 77*.

NOTE In this programming reference, it is assumed that you have a basic knowledge of the SCPI language. For an introduction to SCPI and SCPI programming techniques, refer to:

- The SCPI Consortium: IEEE488.2 Standard Commands for Programmable Instruments, published periodically by various publishers. To obtain a copy of this manual, contact your Agilent representative.

Command Syntax

The Agilent 81250 System does *not* support IEEE 488.2 Common Commands. The device commands for the Agilent 81250 System follow the rules for SCPI Commands.

The name of a command consists of one or more *keywords*. A keyword can have a long or a short form. The short form is denoted in upper case letters.

The following sections highlight some important aspects of the Agilent 81250 command syntax.

Hierarchical Structure

The language used is based on a hierarchical structure (or tree system). Associated commands are grouped together under a common node in the hierarchy. Associated branches and commands are grouped into higher level branches until they meet at the root of the command tree. To obtain a particular command, the full path to it must be specified. This path is constructed by appending keywords to the path as the command tree is descended. Keywords are separated by colons (:). A typical example is:

```
:DVT:INST:LIST?
```

Conventions Used in the Command Reference

The following conventions are used when describing commands and their syntax:

- The command syntax shows the commands as a mixture of upper and lower case letters. The upper case letters indicate the abbreviated spelling for the command. For shorter program lines, you only need to send the abbreviated form. For better program readability, you can send the entire command.
- Square brackets ([]) are used to enclose a keyword that is optional when using the command. Such a node is called a default node.

- Numeric suffixes are represented by (*) in command descriptions.
- Queries are denoted by a question mark (?) at the end of the header.


NOTE The instrument accepts either the abbreviated command form or the entire command form, but not any other forms.

The commands are not case sensitive, so upper or lower case letters or a mix of them are acceptable.

Instrument Commands and Queries Syntax

The instrument command syntax is as follows:

```
<instrument command> ::= <short form mnemonic> [<numeric suffix>]
                        <long form mnemonic> [<numeric_suffix>]
```

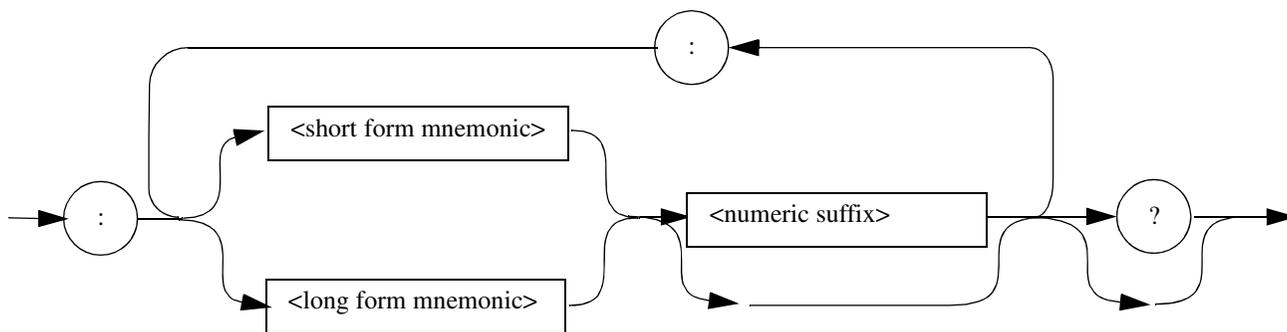

Queries are denoted by a command header with an appended question mark.

```
<instrument command> ::=
    <short form mnemonic> [<numeric suffix>] '?'
    <long form mnemonic> [<numeric_suffix>] '?'
```

Linking Commands

It is possible to link multiple device commands.

To link multiple device commands, use a semicolon and a colon between the commands. Because the Agilent 81250 System allows to configure the available hardware resources as virtual instruments, it is necessary that each individual command sent to the system specifies also the virtual instrument that has to execute the command. This is done by a leading node, the <Handle>. When linking commands, leading nodes can be omitted, as long as they are identical.

Example The following commands could be linked:

```
:_TEST:cgr1:mod2:conn4:puls:del 6e-9  
:_TEST:cgr1:mod2:conn4:puls:width 20e-9  
:_TEST:cgr1:mod2:conn4:puls:tran:lead 5e-9  
:_TEST:cgr1:mod2:conn4:puls:tran:trail 2e-9
```

The linked form would be:

```
:_TEST:cgr1:mod2:conn4:puls:del 6e-9;width 20e-9;  
tran:lead 5e-9;trail 2e-9
```

The Command Tree

The Agilent 81250 SCPI command interface consists of a tree of commands. The branches and sub-branches of this tree are referred to as subsystems. Each subsystem contains a group of related commands.

At the root of the command tree, there are two types of branches (subsystems):

- the DVT subsystem (always available)
- virtual instrument subsystems identified by the handle associated to the instrument

Both are described in *“DVT Subsystem and Virtual Instruments” on page 33*.

Many parameters can be specified on port, terminal and connector level. These aspects are discussed in *“Multiple Parameter Access” on page 34*.

DVT Subsystem and Virtual Instruments

At first—after connecting to the instrument—there is only one subsystem available: the DVT subsystem. The commands in this subsystem provide basic administration features.


The major administrative task is to manage so-called **virtual instruments**. A virtual instrument is a combination of

- a system resource as defined in the dvtsys.txt file
- a software application

With this release of the Agilent 81250, the only application available is the DSR application (Digital Stimulus and Response). Future releases might provide more applications, for example BERT (Bit Error ratio Test).

Virtual instruments can be controlled as if they were separate instruments.

Each virtual instrument is identified by a **handle**. As shown in the following picture, this handle forms the root for a new branch (subsystem) in the command tree. The commands available within this subsystem depend on the selected software application.

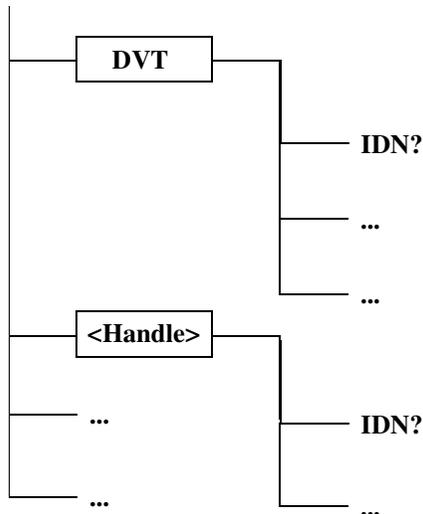

See “*Typical SCPI Programming Sequence*” on page 38 for an example.

NOTE Each virtual instrument has its own error/event queue.

The `<Handle>:SYSTEM:ERROR?` query (see “`<Handle>:SYSTEM:ERROR?`” on page 79) is used to retrieve the next error in the error queue.

Multiple Parameter Access


The command tree provides comfortable means of accessing certain parameters of more than one terminal at a time. According to the system architecture, there are

- **terminals** (DUT input or output pins)
- **ports** (groups of DUT input or output pins with identical or similar properties, such as a data bus)
- **connectors** (input or output connectors of a frontend)


So, for example, if you have a data bus consisting of several terminals, you can group them together in a port, and then set their timing parameters with only one command.

This is shown in the following figure:


CGR(*) :MOD(*) :CONN(*)

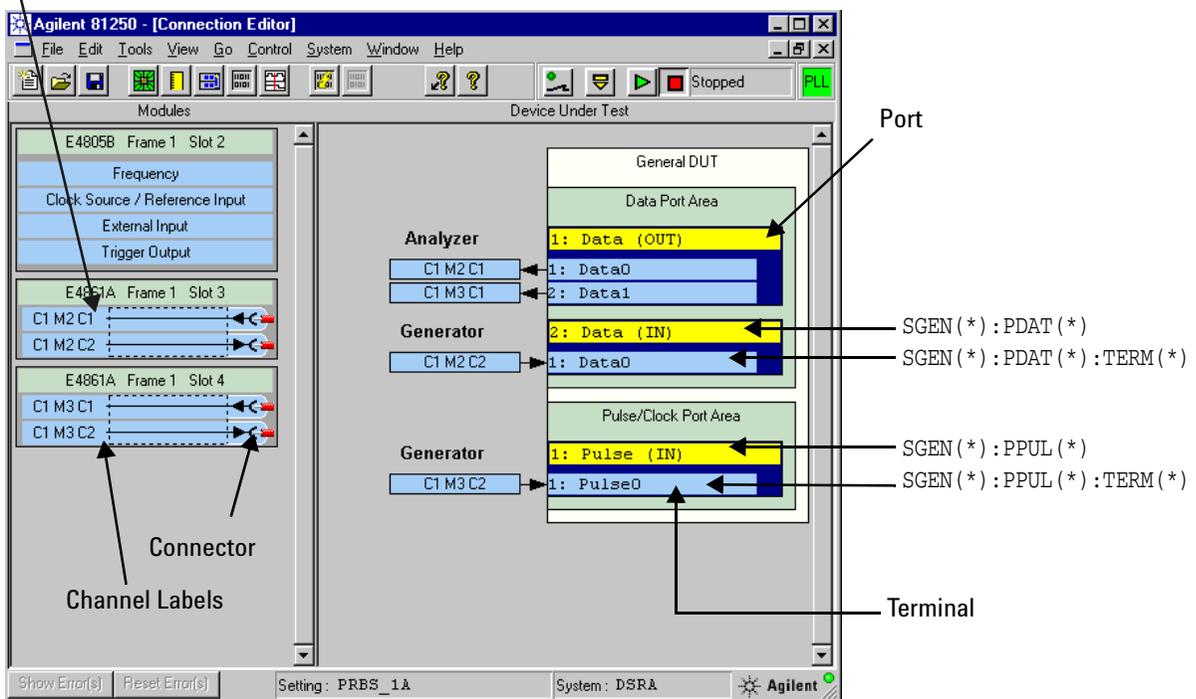

Typical 43.2Gbit Analyzer Commands The following figure shows some typical commands and their corresponding elements for a 43.2Gbit data analyzer system in the Agilent 81250 user interface:

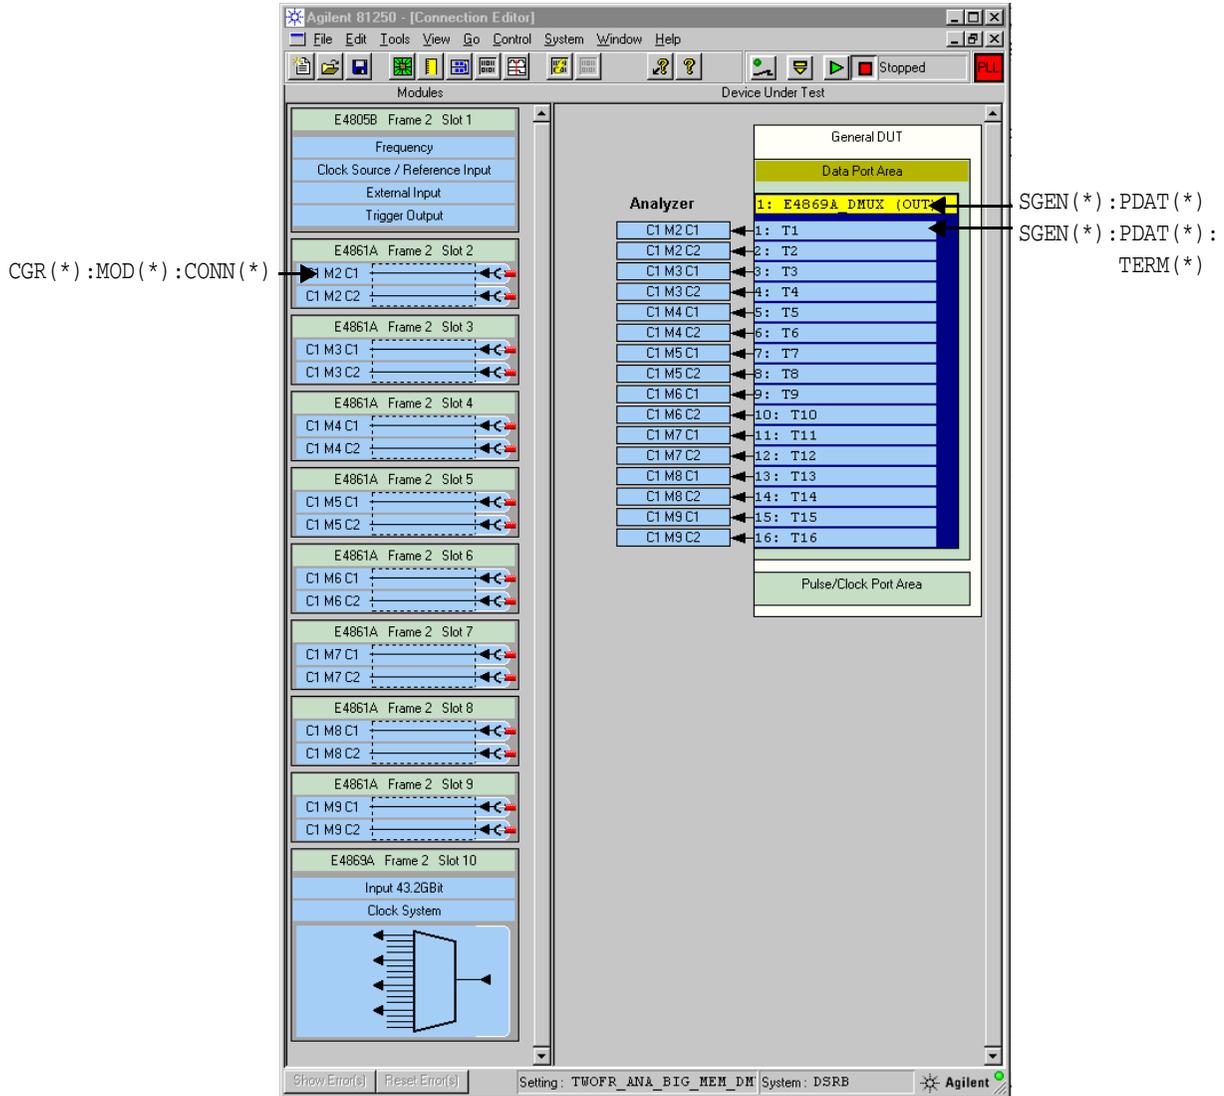

Typical 43.2Gbit Generator Commands The following figure shows some typical commands and their corresponding elements for a 43.2Gbit data generator system in the Agilent 81250 user interface:

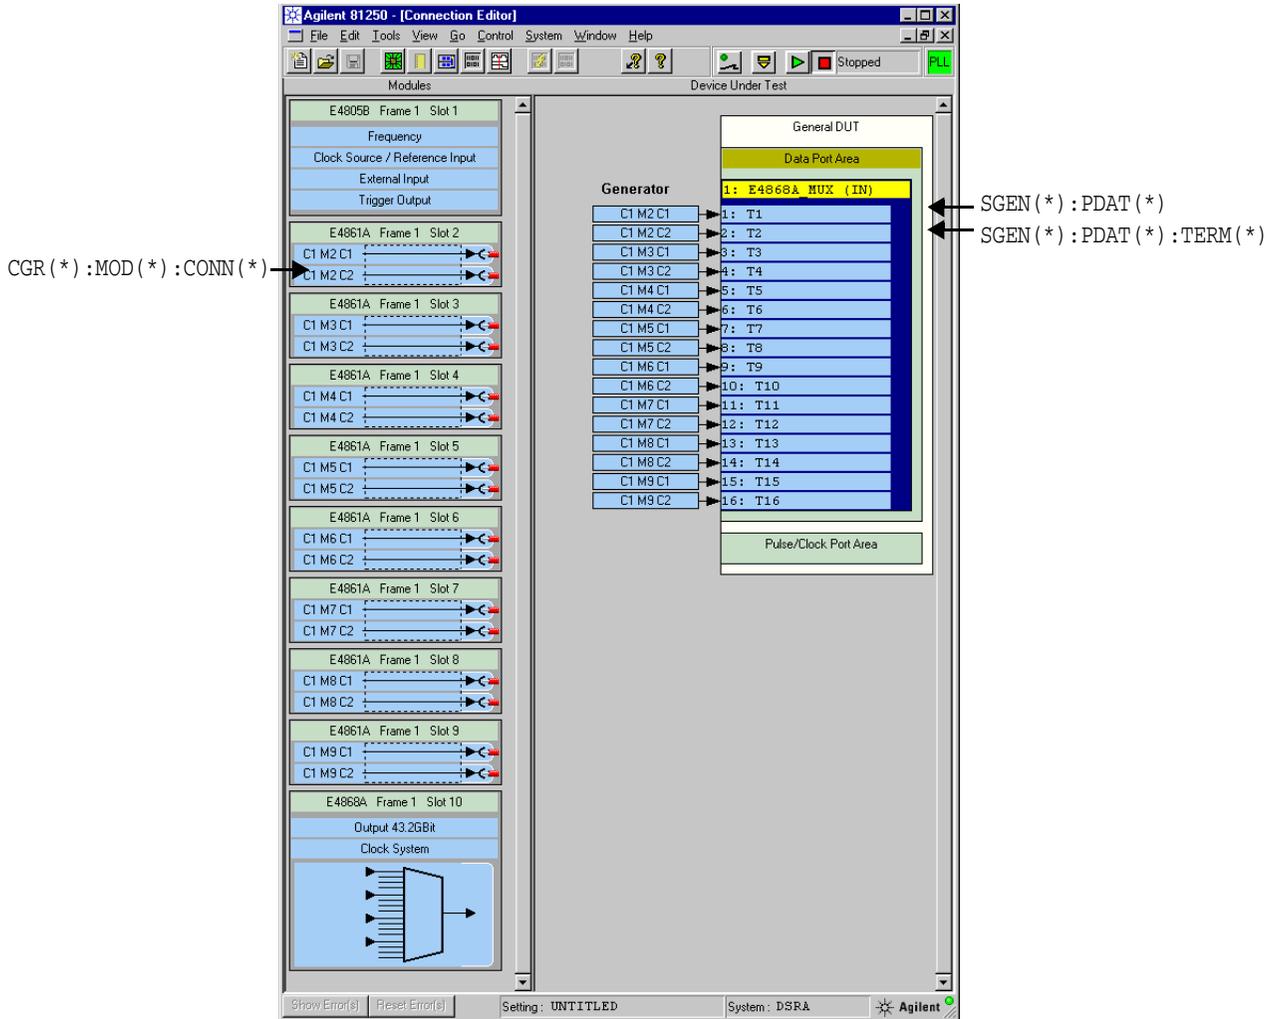

Data ports and pulse ports These figures also show how you can distinguish between data ports (:PDATa(*):) and pulse ports (:PPULSe(*):) on command level.

Types of Parameters The following types of parameters can be accessed on terminal, port, and connector level:

- timing parameters
- level parameters
- output parameters
- input parameters
- format parameters

The corresponding commands are available on each level. In this reference they are described only once, summarized according to the parameter type. The same principle is used for some port, terminal and connector administration commands and for error handling commands.

Example For example, to set the delay for all terminals in a port (for example, pins in a data bus), you can

- either address each terminal individually, using
:SGENeral:PDATA(*):TERMinal(*):PULSe:DELay
- or set the delay for the complete port, using
:SGENeral:PDATA(*):PULSe:DELay

Both commands are described in “:PULSe:DELay” on page 185.

Example Programs

Two example programs are discussed in the following:

- “*Typical SCPI Programming Sequence*” on page 38 shows a typical sequence of SCPI commands used for programming the Agilent 81250.
- “*Example C++ Program*” on page 40 guides you through an example program and a class library supplied with the Agilent 81250.

Typical SCPI Programming Sequence

When implementing programs for the Agilent 81250 using SCPI commands, you should keep to the following sequence:

1. Create instrument
2. Set system parameters
3. Create model of DUT
4. Connect DUT to instrument
5. Set signal parameters
6. Create sequence
7. Run test
8. Destroy instrument

NOTE Always make sure that you destroy the handle at the end of your program.

Here is a little example program showing some of these steps.

```
:DVT:INST:RES:LIST? "DSR"      # Ask what DSR instruments are
                                # pre-configured in the
                                # System (see
                                # d:\81200\cfg\dvtsys.txt file)
                                # Returns: "DSRA", "DSRB"

                                # Create a handle, better ask for a
                                # handle: give TEST as a suggestion
                                # for the handle:

:DVT:INST:HAND:CRE? TEST, "DSR", "DSRA"

                                # When the suggested handle is not
                                # used, then the system will return:
                                # _TEST

:_TEST:SGEN:GLOB:PER 50e-9     # set period:
```

```

:_TEST:SGEN:GLOB:MUX 1      # set system BLG factor, check that
                             # period and memory depth match:
                             # set an input data port named
                             # AddrBus with 4 Terminals:

:_TEST:SGEN:PDAT:APP "INPUT_PORT", 4, "AddrBus"

                             # add a 5th terminal with name
                             Addr4:

:_TEST:SGEN:PDAT1:TERM5:APP "Addr4", 5

                             # connect terminal 1 of port AddrBus
                             # to connector 1 of module 2:

:_TEST:SGEN:CONN:PDAT1:TERM1:TO (@0102001)

                             #set pulse width of terminal 1 (T1):

:_TEST:SGEN:PDAT1:TERM1:PULS:WIDT 20e-9

                             # set delay of T1:

:_TEST:SGEN:PDAT1:TERM1:PULS:DEL 5e-9

                             # set leading edge of T1:

:_TEST:SGEN:PDAT1:TERM1:PULS:TRANS 1e-9

                             # set high level of T1:
                             # High level has to be higher than
                             # the actual low level.

:_TEST:SGEN:PDAT1:TERM1:VOLT:HIGH 3

                             # set low level of T1:

:_TEST:SGEN:PDAT1:TERM1:VOLT:LOW 1

                             # set load impedance for T1:

:_TEST:SGEN:PDAT1:TERM1:OUTP:IMP:EXT 50

:_DVT:INST:HAND:DEST _TEST  # When the virtual device is no
                             # longer required, the handle can be
                             # eliminated:

```

Example C++ Program

This example is intended to show the more sophisticated steps of analyzing the system configuration and setting up the system as required, importing segment data, and running a measurement in “compare and acquire around error” mode. Furthermore, the Edit subsystem is used to handle the captured data.

The example program is divided into “*The main() Procedure*” on page 41 and “*The doIt() Procedure*” on page 41. The program uses a small interface class (see “*The lib.cpp Interface Class Library*” on page 40) that provides methods for initializing the system, dealing with handles, executing the SCPI commands, and logging errors.

By default, the files with the example code (main.cpp, lib.cpp, and lib.h) can be found in the Agilent 81250 installation directory:

```
C:\Program Files\Agilent\Agilent 81200\samples\ecap
```

The lib.cpp Interface Class Library

The file lib.cpp defines the HP 81200 class, which is an interface class to the Agilent 81250 system. The class itself uses the “*Agilent 81250 String Interface Library*” on page 22.

For a complete listing, refer to “*Lib.cpp Interface Class Library Code*” on page 351.

The class provides the following public methods:

- Init()

The Init() method connects to an Agilent 81250 server on the local machine or to a specified server. It creates a handle for the specified system. This handle is only used within the class. An extra parameter specifies a file to be used for error logging.

- Exit()

The Exit() method releases the handle and disconnects from the system.

- Call()

There are two Call() methods, distinguished by the number of parameters: one to execute SCPI commands, one to execute SCPI queries.

Both methods return “false” in case of an error. The query method features an additional parameter to return the result of the query.

The main() Procedure

The file `main.cpp` contains the application-specific code. It uses the `lib.cpp` interface class to communicate with the Agilent 81250 system.

For a complete listing, refer to “*Main.cpp Application Code*” on page 356.

The `main()` procedure implements the following steps:

- Creates an HP 81200 object and calls the `Init()` method to create a handle and to connect to the system. `stdout` is used for error logging.
- Invokes the `doIt()` procedure, which prepares and executes all required SCPI commands.
- Calls the `Exit()` method to release the handle and to disconnect from the system.

The doIt() Procedure

The code for the `doIt()` procedure is part of the file `main.cpp`. It prepares and executes all SCPI commands required for this example.

For a complete listing, refer to “*Main.cpp Application Code*” on page 356.

These are the most important steps performed by the `doIt()` procedure:

- Stops and resets the system.
- Analyzes the system configuration.

To create a list of all analyzers and generators, the numbers of clock groups, modules within each clock group, and connectors within each module are determined.

In loops over all clock groups, modules, and connectors, the type of each connector is determined. The connectors are appended to the list of analyzers or to the list of exercisers.

- Connects generators and analyzers to one port each.

The number of generators (aGenCnt) and the list of generators (aGenerators) are used to create an input port with the required number of terminals. The terminals are connected to the generator channels, starting at terminal 1.

Number and list of analyzers (aAnaCnt and aAnalyzers) are used to create and connect output port and terminals.

This step only makes sense for this example. In real life you know the number of terminals and ports required by the DUT and set up the Agilent 81250 accordingly.

- Switches on all generator and analyzer ports, and applies levels and thresholds.

- Imports segment data from the file walk64.txt.

- Sets the period.

- Sets up a sequence that uses the imported segment.

First the number of available loop levels is determined (depending on the clock module used).

The highest loop level is used to set up an infinite loop. The imported segment is used as data for the sequence.

The start of the sequencer is used to generate a trigger signal at the trigger output.

- Sets measurement mode to “compare and acquire around error”

- Saves the setting for later use.

- Starts the measurement.

- Waits until the measurement is done (only works online).

- Stops the measurement.

- Exports the captured data and the error memory.

This demonstrates how the :EDIT:SEGMENT(*) subsystem can be used to handle captured data.

First, the segments are opened and information on the coding used for the captured data is queried. Then the captured data are printed trace by trace.

Finally, the segments are saved, exported, and closed.

SCPI Commands Overview

This section provides an application-oriented overview of the SCPI commands available in the DVT subsystem and in the subsystems for DSR applications.

The following categories are available:

- *“Generic Administration Commands” on page 44*
- *“Virtual Instruments Administration Commands” on page 44*
- *“Mass Memory Commands” on page 45*
- *“Segment Editing Commands” on page 46*
- *“Global Commands” on page 48*
- *“Clock Reference Input Commands” on page 49*
- *“External Input Commands” on page 50*
- *“Trigger Output Commands” on page 50*
- *“Port Administration Commands” on page 51*
- *“Terminal Administration Commands” on page 52*
- *“Connector Administration Commands” on page 52*
- *“Clockgroup Administration Commands” on page 53*
- *“Sequence Commands” on page 53*
- *“Synchronization Commands” on page 54*
- *“Analyzer Commands” on page 55*
- *“Level Parameter Commands” on page 55*
- *“Amplitude/Offset Correction Factor Commands” on page 56*
- *“Timing Parameter Commands” on page 57*
- *“MUX Parameter Commands” on page 58*
- *“DeMUX Parameter Commands” on page 59*
- *“DeMUX Rewiring Commands” on page 59*
- *“Delay Control Parameter Commands” on page 60*
- *“Output Parameter Commands” on page 63*
- *“Optical Output Commands” on page 64*

- “Input Parameter Commands” on page 60
- “Performance Parameter Commands” on page 66
- “Format Parameter Commands” on page 66

Generic Administration Commands

Command (Link to detailed description)	Description
<code>":DVT:IDN?"</code> on page 69	Returns the device identity.
<code>":DVT:SYSTem:ERRor?"</code> on page 70	Returns the first entry of the error queue.
<code>":DVT:INSTrument:LIST?"</code> on page 71	Returns a comma-separated list of items containing the names of all applications.
<code>":DVT:INSTrument:RESource:LIST?"</code> on page 71	Returns a list of available systems names. A system name can be used to create an association between a set of modules (system) and an application software to build an virtual instrument.
<code>":DVT:INSTrument:HANDle:CREate?"</code> on page 72	Creates a handle for a new virtual instrument.
<code>":DVT:INSTrument:HANDle:LIST?"</code> on page 73	Returns a list of all virtual instrument handles.
<code>":DVT:INSTrument:HANDle:DESTroy?"</code> on page 73	Destroys the handle for a virtual instrument and frees all resources.

Virtual Instruments Administration Commands

Command (Link to detailed description)	Description
<code>":<Handle>:IDN?"</code> on page 78	Returns the device identity.
<code>":<Handle>:OPC?"</code> on page 78	The query returns when all modules report that they are ready.
<code>":<Handle>:SYSTem:ERRor?"</code> on page 79	Returns the first entry of the error queue.
<code>":<Handle>:SYSTem:CINformation?"</code> on page 80	Returns the configuration information of an Agilent 81250 system.
<code>":<Handle>:SYSTem:CLient[:HANDle]?"</code> on page 84	Returns the name of the virtual instrument currently connected to the server.
<code>":<Handle>:SYSTem:CLient:LOCK" on page 84</code>	Used to take over the control of the virtual instrument explicitly.
<code>":<Handle>:SYSTem:CLient:BLOCK" on page 85</code>	Used to take over the control of the virtual instrument explicitly. Other clients will be blocked until the instrument is unlocked.
<code>":<Handle>:SYSTem:CLient:UNLock" on page 85</code>	Used to “unlock” or to “set free” the virtual instrument.
<code>":<Handle>:CONFIguration:CGRoups(*)?"</code> on page 86	Returns the number of clock groups that are available in the system.
<code>":<Handle>:CONFIguration:CGRoups(*):MODules(*)?"</code> on page 86	Returns the number of modules that are available in a clock group.

Command (Link to detailed description)	Description
<i>":<Handle>:CONFIguration:CGRoups(*):MODules(*):CONNectors(*)" on page 87</i>	Returns the number of connectors of a module.
<i>":<Handle>:CONFIguration:CGRoups(*):MODules(*):CONNectors(*):TYPE?" on page 87</i>	Returns the type of the connector.
<i>":<Handle>[:CGRoup(*):CINformation?" on page 124</i>	Returns the clock group configuration information.
<i>":<Handle>[:CGRoup(*):MODule(*):CINformation?" on page 126</i>	Returns the module configuration information.
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):CINformation?" on page 129</i>	Returns the connector configuration information.
<i>":<Handle>:CONFIguration:STYPes?" on page 87</i>	Returns a list of Scheme TYPes supported by the Agilent 81250 System.
<i>":<Handle>:CONFIguration:PROFile[:VALue]" on page 88</i>	Sets a profile parameter to a specified value.
<i>":<Handle>:CONFIguration:PROFile[:VALue]?" on page 88</i>	Returns an expression containing the value of a profile parameter.
<i>":<Handle>:CONFIguration:PROFile:REMOve" on page 88</i>	Removes the specified parameter from the profile.
<i>":<Handle>:CONFIguration:PROFile:LIST?" on page 89</i>	Lists the parameters contained in the profile.
<i>":<Handle>:SYSTem:TEST:MODule" on page 81</i>	Starts a module selftest. The results of this test are stored in the message queue.
<i>":<Handle>:SYSTem:TEST:GLOBal" on page 82</i>	Starts a system-wide selftest. The results of this test are stored in the message queue.
<i>":<Handle>:MODule:SREVisions" on page 82</i>	Checks the actual BIOS Software revisions against the expected revision located in the firmware.
<i>":<Handle>:SYSTem:MQUeue[:READ]?" on page 83</i>	Returns the first item contained in the message queue.
<i>":<Handle>:SYSTem:MQUeue:LENGth?" on page 83</i>	Returns the length of the message queue.
<i>":<Handle>:SYSTem:PON[:STATus]" on page 83</i>	Moves the messages, which are generated by the modules at system start up, to the message queue.
<i>":<Handle>:SGENeral:INformation:PCLasses?" on page 141</i>	Returns the list of implemented port classes in a comma separated quoted string list.

Mass Memory Commands

Command (Link to detailed description)	Description
<i>":<Handle>:MMEMory:LIST?" on page 90</i>	Returns an expression containing a comma separated list of quoted strings. Each string contains one element found in the directory <"Absolute Path">.
<i>":<Handle>:MMEMory:INformation?" on page 91</i>	Returns detailed information about the specified object.
<i>":<Handle>:MMEMory:SEGment:LOAD" on page 92</i>	Loads new segments into or updates segments in the Agilent 81250 System's database
<i>":<Handle>:MMEMory:SEGment:SAVE" on page 93</i>	Stores segments to file.
<i>":<Handle>:MMEMory:SEGment:GET?" on page 94</i>	Returns an expression that contains the contents of segment(s) (vector definition).
<i>":<Handle>:MMEMory:SETting:NAME?" on page 94</i>	Returns the current setting name.

Command (Link to detailed description)	Description
<i>":<Handle>:MMEMory:SETting:LOAD" on page 95</i>	Loads the current setting or a specified setting into the Agilent 81250 System's database.
<i>":<Handle>:MMEMory:SETting:SAVE" on page 95</i>	Saves changes either into the current setting or into a new setting.
<i>":<Handle>:MMEMory:SETting:NEW" on page 96</i>	Performs a reset and creates an "untitled" segment.
<i>":<Handle>:MMEMory:SETting:DELeTe" on page 96</i>	Deletes a specified setting from the Agilent 81250 System's database.
<i>":DVT:MMEMory:SETting:IMPort" on page 75</i>	Allows to import a setting into the Agilent 81250 System.
<i>":SETting:IMPort:DVT:MMEMory:SETting:EXPort" on page 74</i>	Exports a setting into a newly created file.
<i>":DVT:MMEMory:SETting:EXPort?" on page 74</i>	Returns the setting data that would normally be written to a file.

Segment Editing Commands

Command (Link to detailed description)	Description
<i>":<Handle>:EDIT:SEGMENT(*):CREate?" on page 100</i>	Creates a new segment.
<i>":<Handle>:EDIT:SEGMENT(*):OPEN?" on page 98</i>	Opens the specified segment.
<i>":<Handle>:EDIT:SEGMENT(*):SAVE" on page 99</i>	Saves the changes made to the current segment name, or creates a new segment name.
<i>":<Handle>:EDIT:SEGMENT(*):CLoSe" on page 103</i>	Closes the segment editor specified by the segment inspector index number without saving possible changes made to the current segment name.
<i>":<Handle>:EDIT:SEGMENT(*):DELeTe" on page 100</i>	Deletes the specified segment.
<i>":<Handle>:EDIT:SEGMENT(*):EXISts?" on page 101</i>	Checks whether the specified segment name is located in the Agilent 81250 System's database.
<i>":<Handle>:EDIT:SEGMENT(*):RPAth?" on page 102</i>	Returns the absolute path for one segment.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:CODing?" on page 107</i>	Returns the segments coding.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:CODing" on page 106</i>	Sets a segment's coding.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:ERRor:FIRSt?" on page 107</i>	Returns the coordinates (trace, vector) of the first found error.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:ERRor:NEXt?" on page 108</i>	Returns the coordinates (trace, vector) of the first found error, starting at the given coordinates.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:ERRor:PREVious?" on page 108</i>	Returns the coordinates (trace, vector) of the first found error, starting at the given coordinates, searching backwards.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:FIND:FIRSt?" on page 109</i>	Returns the coordinates (trace, vector) of the first found instance of the given pattern.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:FIND:NEXt?" on page 111</i>	Returns the coordinates (trace, vector) of the first found instance of the given pattern, starting at the given coordinates.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:FIND:PREVious?" on page 111</i>	Returns the coordinates (trace, vector) of the first found instance of the given pattern, starting at the given coordinates, searching backwards.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:DATA" on page 103</i>	Creates a state range and fills it with the required pattern.
<i>":<Handle>:EDIT:SEGMENT(*):PATtern:DATA?" on page 104</i>	Returns from the segment inspector the vector stream bounded by the specified rectangle.

Command (Link to detailed description)	Description
<i>":<Handle>:EDIT:SEGMent(*):PATtern:LENGth?" on page 112</i>	Returns the numbers of vectors of a segment.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:WIDTh?" on page 112</i>	Returns the numbers of traces of a segment.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:COpy" on page 113</i>	Copies the bounded rectangle of data from the segment into the clipboard.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:PASTE" on page 113</i>	Pastes the data currently stored in the clipboard to the specified segment.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:FILL" on page 114</i>	Sets the bounded area of the segment with the same state value.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:INVert" on page 115</i>	Inverts the states information in the bounded area.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:MIRRor" on page 116</i>	Rotates the specified block about horizontal (VECTor) or vertical axis (TRACe).
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:INSert" on page 117</i>	Inserts new traces or vectors into a segment.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:DELeTe" on page 117</i>	Deletes traces or vectors from a segment.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:CONVerse" on page 118</i>	Changes the current coding for the segment and converts existing data in the segment according to the specified mapping
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:SERialize" on page 119</i>	Serializes a parallel data stream.
<i>":<Handle>:EDIT:SEGMent(*):PATtern:MODify:DESERialize" on page 120</i>	Deserializes a serial data stream.
<i>":<Handle>:EDIT:SEGMent(*):PARAMeter:LENGth?" on page 120</i>	Gets the length of the list of parameters available for this segment.
<i>":<Handle>:EDIT:SEGMent(*):PARAMeter:LIST?" on page 121</i>	Gets the list of parameters available for this segment.
<i>":<Handle>:EDIT:SEGMent(*):PARAMeter[:VALue]?" on page 121</i>	Returns the value for a specified parameter from the segment.
<i>":<Handle>:EDIT:SEGMent(*):PARAMeter[:VALue]" on page 122</i>	Sets the value for a specified parameter in the segment.
<i>":<Handle>:EDIT:SEGMent(*):PARAMeter:REMOve" on page 122</i>	Removes a parameter from the list of parameters in the segment.
<i>":<Handle>:EDIT:SEGMent(*):TYPE" on page 122</i>	Sets the segment type for the current segment.
<i>":<Handle>:EDIT:SEGMent(*):TYPE?" on page 123</i>	Returns the segment type of the segment specified by the segment inspector index number.

Global Commands

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:INITiate:CONTinuous" on page 154</i>	Starts/stops the system.
<i>":<Handle>:SGENeral:GLOBal:INITiate:CONTinuous?" on page 154</i>	Returns the current state of the system.
<i>":<Handle>:SGENeral:GLOBal:SYSTem:STATe?" on page 155</i>	Returns the current state of the system.
<i>":<Handle>:SGENeral:GLOBal:CALibration:PUSe PASSive" on page 143</i>	Sets deskew to using passive probe.
<i>":<Handle>:SGENeral:GLOBal:CALibration:SELF DELay" on page 143</i>	Autocalibrates the system after any frontend have been exchanged.
<i>":<Handle>:SGENeral:GLOBal:PERiod" on page 144</i>	Sets the period of the Agilent 81250 System.
<i>":<Handle>:SGENeral:GLOBal:PERiod?" on page 145</i>	Returns the period of the Agilent 81250 System.
<i>":<Handle>:SGENeral:GLOBal:FREQuency" on page 145</i>	Sets the frequency of the Agilent 81250 System.
<i>":<Handle>:SGENeral:GLOBal:FREQuency?" on page 145</i>	Returns the frequency of the Agilent 81250 System.
<i>":<Handle>:SGENeral:GLOBal:MUX" on page 146</i>	Defines the global settings for the Segment Resolution.
<i>":<Handle>:SGENeral:GLOBal:MUX?" on page 146</i>	Returns the current MUX factor (Segment Resolution).
<i>":<Handle>:SGENeral:GLOBal:DOFFset" on page 143</i>	Specifies an offset value to the fixed delay for all connectors.
<i>":<Handle>:SGENeral:GLOBal:DOFFset?" on page 144</i>	Returns the currently set delay offset.
<i>":<Handle>:SGENeral:GLOBal:CONNect" on page 142</i>	Connects or disconnects all enabled connectors of the Agilent 81250 System.
<i>":<Handle>:SGENeral:GLOBal:CONNect?" on page 142</i>	Returns the actual connection status of the enabled connectors.
<i>":<Handle>:SGENeral:GLOBal:PLL:DSState?" on page 149</i>	Determines the PLL (Phase Locked Loop) state and returns a list of unlocked modules.
<i>":<Handle>:SGENeral:GLOBal:PLL:STATe?" on page 150</i>	Determines the PLL (Phase Locked Loop) state.
<i>":<Handle>:SGENeral:GLOBal:FETCh:ERRor:ANY?" on page 144</i>	Reports whether there has been found any error.

Clock Reference Input Commands

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]" on page 173</i>	Sets the clock reference or the external clock mode.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]?" on page 174</i>	Returns the actual status of the Clock/Reference Input of the Central resource.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDRList?" on page 174</i>	Returns the list of channels that have CDR (Clock Data Recovery) capabilities.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDR" on page 174</i>	Sets the channel that recovers the clock from the data stream.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDR?" on page 175</i>	Returns the channel that recovers the clock from the data stream.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:VALue?" on page 175</i>	Measures and returns the supplied external clock at the clock input of the E4805B or E4808A central module.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MEASurement[:DIRect]" on page 175</i>	Measures the external clock and sets the corresponding mode.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MULTIplier" on page 176</i>	Sets the clock multiplier.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MULTIplier?" on page 176</i>	Returns the current clock multiplication factor.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:RCLOCK:DETECT" on page 177</i>	Measures the external clock reference and sets the corresponding mode automatically.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MEASurement" on page 177</i>	Measures the external clock and sets the corresponding mode EXTERNAL automatically.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:TVOLTage" on page 178</i>	Specifies the termination voltage.
<i>":<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:TVOLTage?" on page 178</i>	Returns the actual setting of the termination voltage.

External Input Commands

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:ARM[:SEQuence][:LAYer][:SOURce]" on page 180</i>	Controls the start mode of the Agilent 81250 System.
<i>":<Handle>:SGENeral:GLOBal:ARM?" on page 181</i>	Returns the actual status of the External Input connector at the front of the Central resource.
<i>":<Handle>:SGENeral:GLOBal:ARM[:SEQuence][:LAYer]:SENSe" on page 181</i>	Specifies the input level condition which is used in the GATed STARtsignal STOPsignal modes.
<i>":<Handle>:SGENeral:GLOBal:ARM[:SEQuence][:LAYer]:SENSe?" on page 181</i>	Returns the actual setting of the input level condition for the gate or start/stop signal.
<i>":<Handle>:SGENeral:GLOBal:ARM[:SEQuence][:LAYer]:THReshold" on page 182</i>	Specifies the threshold of the external input signal which is used in the GATed STARtsignal STOPsignal modes.
<i>":<Handle>:SGENeral:GLOBal:ARM[:SEQuence][:LAYer]:THReshold?" on page 182</i>	Returns the actual threshold for the external input signal used in the gate or start/stop mode.
<i>":<Handle>:SGENeral:GLOBal:ARM[:SEQuence][:LAYer]:TVOLtage" on page 182</i>	Specifies the termination voltage of the external input signal which is used in the GATed STARtsignal STOPsignal modes.
<i>":<Handle>:SGENeral:GLOBal:ARM[:SEQuence][:LAYer]:TVOLtage?" on page 183</i>	Returns the actual termination voltage for the external input signal used in the gate or start/stop mode.

Trigger Output Commands

Command (Link to detailed description)	Description
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:DELay" on page 134</i>	Varies the delay of the trigger output signal.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:DELay?" on page 134</i>	Returns the current delay of the trigger output signal.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:MUX" on page 135</i>	Sets the frequency multiplier factor for the individual connector.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:MUX?" on page 135</i>	Returns the MUX factor associated with the trigger output.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:OUTPut[:STATe]" on page 135</i>	Sets the state of the trigger output of an E4809A clock module.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:OUTPut[:STATe]?" on page 136</i>	Returns the state of the trigger output of an E4809A clock module.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:VOLtage[:LEVel][:IMMediate]:HIGH" on page 136</i>	Sets the high voltage level of the trigger output signal.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:VOLtage[:LEVel][:IMMediate]:HIGH?" on page 136</i>	Returns the high voltage level of the trigger output signal.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:VOLtage[:LEVel][:IMMediate]:LOW" on page 137</i>	Sets the low voltage level of the trigger output signal.
<i>":<Handle>[:CGRoup(*)][[:SOURce]:TRIGger:VOLtage[:LEVel][:IMMediate]:LOW?" on page 137</i>	Returns the low voltage level of the trigger output signal.

Command (Link to detailed description)	Description
<i>":<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:TVOLTage" on page 137</i>	Specifies the termination voltage of a trigger output connector.
<i>":<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:TVOLTage?" on page 138</i>	Returns the current termination voltage of the trigger output connector.
<i>":<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:IMPedance:EXternal" on page 138</i>	Specifies the external termination IMPedance.
<i>":<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:IMPedance:EXternal?" on page 138</i>	Returns the current programmed external termination impedance (load impedance).
<i>":<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:MODE" on page 139</i>	Selects the source of the trigger output.
<i>":<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:MODE?" on page 139</i>	Returns the actual source used for the trigger signal.

Port Administration Commands

The following table lists the commands available for the administration of pulse and data ports.

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:INformation:PClasses?" on page 141</i>	Returns the list of implemented port classes in a comma separated quoted string list.
<i>":APPend" on page 300</i>	Creates and appends a new port to the list of ports.
<i>":LIST?" on page 301</i>	Returns a comma-separated list of port names.
<i>":ATYPes?" on page 301</i>	Returns a comma-separated list of available predefined port TYPES.
<i>":DELeTe" on page 301</i>	Deletes the port specified by the suffix of PPULse.
<i>":REName" on page 302</i>	Renames the port specified by the suffix of PPULse.
<i>":NAME?" on page 302</i>	Returns the name of the specified port.
<i>":NUMBer?" on page 302</i>	Returns the number of the specified port.
<i>":TYPE?" on page 303</i>	Returns the type of the specified port.
<i>":MUX" on page 201</i>	Sets the frequency multiply factor (MUX factor) for the specified port.
<i>":MUX?" on page 201</i>	Returns the current frequency multiply factor (MUX factor) for the specified port.
<i>":OUTPut:IMPedance:EXternal" on page 273</i>	Sets the external termination impedance
<i>":OUTPut:IMPedance:EXternal?" on page 273</i>	Returns the currently programmed value for the termination (load) impedance for the connectors of the specified port.
<i>":CALibration:CDElay" on page 303</i>	Sets a cable delay for the specified port, to synchronize the signals at the DUT terminals.
<i>":CALibration:CDElay?" on page 303</i>	Returns the current cable delay for the specified port.
<i>":SPECies?" on page 304</i>	Returns the species (electrical or optical) of the specified port.

Terminal Administration Commands

The following table lists the commands available for administration of pulse and data port terminals.

Command (Link to detailed description)	Description
<i>":APPend" on page 305</i>	Creates and appends a new terminal to the list of terminals.
<i>":LIST?" on page 305</i>	Returns a comma-separated list of terminal names.
<i>":DELeTe" on page 306</i>	Deletes the terminal specified by the suffix of TERMIal.
<i>":FETch:SStatus?" on page 306</i>	Returns the status of the specified terminal.
<i>":REName" on page 306</i>	Renames the terminal specified by the suffix of TERMIal.
<i>":NAME?" on page 307</i>	Returns the name of the specified terminal.
<i>":TYPE?" on page 307</i>	Returns the type of the specified terminal.
<i>":MOVE" on page 307</i>	Moves the specified terminal to a new position.
<i>":CALibration:CDELaY" on page 308</i>	Sets a cable delay for the specified terminal in the specified port to synchronize the signals at the DUT terminals.
<i>":CALibration:CDELaY?" on page 308</i>	Returns the current cable delay for the specified terminal in the specified port.

Connector Administration Commands

Command (Link to detailed description)	Description
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):CINformation?" on page 129</i>	Returns the connector configuration information.
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):TYPE?" on page 130</i>	Returns the product number of the frontend to which the connector belongs.
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):NAME?" on page 130</i>	Returns the name of this connector.
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):TNAME?" on page 130</i>	Returns the Terminal NAME to which this connector is connected.
<i>":REMove" on page 309</i>	Disconnects all terminals within the specified port or terminal.
<i>":TERMIal(*):[TO]" on page 310</i>	Connects the specified terminal to the specified channel or channels.
<i>":TERMIal(*):[TO]?" on page 311</i>	Returns the channel to which the specified terminal is connected.
<i>":MUX" on page 201</i>	Sets the MUX factor associated with this connector.
<i>":MUX?" on page 201</i>	Returns the MUX factor associated with this connector.
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):CALibration:CDELaY" on page 131</i>	Sets a cable delay for the specified connector to synchronize it with other signal applied to the DUT terminals.
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):CALibration:CDELaY?" on page 131</i>	Returns the current cable delay for the specified connector of a specific module.
<i>":<Handle>[:CGRoup(*):MODule(*):CONNector(*):CALibration:ZDELaY" on page 131</i>	Sets a zero delay for the specified connector of a specific the Agilent 81250 System's module.

Command (Link to detailed description)	Description
<code>":<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):CALIBRATION:ZDELAY?"</code> on page 132	Returns the current zero delay for the specified connector.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):SPECIES[:VALUE]?"</code> on page 132	Returns a comma-separated list of the species states that are supported by the connector.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):SPECIES:STATE" on page 132</code>	Switches the connector into either electrical (ELEC) or optical (OPT) mode.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):CONNECTOR(*):SPECIES:STATE?" on page 133</code>	Returns the current species of the connector.
<code>":OUTPUT:IMPEDANCE:EXTERNAL" on page 273</code>	Specifies the external termination impedance.
<code>":OUTPUT:IMPEDANCE:EXTERNAL?" on page 273</code>	Returns the currently programmed external termination impedance (load impedance).

Clockgroup Administration Commands

Command (Link to detailed description)	Description
<code>":<Handle>[:CGROUP(*)]:CINFORMATION?" on page 124</code>	Returns the clock group configuration information.
<code>":<Handle>[:CGROUP(*)]:MCLOCK:SOURCE[:VALUE]" on page 125</code>	Controls which of the clock modules generates the "master" clock.
<code>":<Handle>[:CGROUP(*)]:MCLOCK:SOURCE:VALUE?" on page 125</code>	Returns the state of the clock module specified.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):CINFORMATION?" on page 126</code>	Returns the module configuration information.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):TYPE?" on page 127</code>	Returns the product number in a quoted string.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):SLOT?" on page 127</code>	Returns the slot number in which the module is located.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):FRAME?" on page 127</code>	Returns the frame number to which this module belongs.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):NAME?" on page 127</code>	Returns the name of this module.
<code>":<Handle>[:CGROUP(*)]:MODULE(*):CNAMES?" on page 128</code>	Returns a quoted list of Connector names.

Sequence Commands

Command (Link to detailed description)	Description
<code>":<Handle>:SGENERAL:GLOBAL:SEQUENCE[:VALUE]" on page 157</code>	Loads a data sequence in the form of an expression into the system.
<code>":<Handle>:SGENERAL:GLOBAL:SEQUENCE[:VALUE]?" on page 161</code>	Returns the current data sequence of the system.
<code>":<Handle>:SGENERAL:GLOBAL:SEQUENCE:EVENTS" on page 162</code>	Defines events for the system.

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:SEQuence:EVENTs?" on page 164</i>	Returns a list of events defined for the system.
<i>":<Handle>:SGENeral:GLOBal:SEQuence:FORCe" on page 165</i>	Downloads the actual sequence immediately.
<i>":<Handle>:SGENeral:GLOBal:SEQuence:LLEVel?" on page 165</i>	Returns the actually available loop levels.
<i>":<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol" on page 166</i>	Sets the value of the program control event.
<i>":<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol?" on page 166</i>	Returns the value of the program control event.
<i>":<Handle>:SGENeral:GLOBal:SEQuence:STATe?" on page 166</i>	Returns the number of the currently executed block.

Synchronization Commands

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:USED?" on page 168</i>	Returns whether a synchronization flag is found in the programmed sequence.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:BERThreshold" on page 168</i>	Sets the threshold for the bit error ratio to be accepted during synchronization.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:BERThreshold?" on page 169</i>	Returns the currently set bit error ratio threshold.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:SMODE" on page 169</i>	Specifies how the synchronization of the analyzers is achieved.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:SMODE?" on page 170</i>	Returns the currently set synchronization mode.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:APSelect" on page 170</i>	Sets the state of the Automatic Polarity Select feature.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:APSelect?" on page 171</i>	Returns the state of the Automatic Polarity Select feature.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:APAAlignment" on page 171</i>	Specifies whether an automatic phase optimization is done after a synchronization in infinite range.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:APAAlignment?" on page 172</i>	Returns whether an automatic phase optimization is done after a synchronization in infinite range.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:PACCuracy" on page 172</i>	Specifies how accurate the phase optimization is done after a synchronization in infinite synchronization range.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:PACCuracy?" on page 172</i>	Returns the required phase optimization accuracy.

Analyzer Commands

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:CONFigure?" on page 151</i>	Returns the last measurement mode setting in a quoted string.
<i>":<Handle>:SGENeral:GLOBal:CONFigure:CAPture" on page 151</i>	Activates the Capture measurement mode.
<i>":<Handle>:SGENeral:GLOBal:CONFigure[:ECOut]" on page 152</i>	Activates the Error Rate measurement mode.
<i>":<Handle>:SGENeral:GLOBal:CONFigure:ECAPture" on page 152</i>	Activates the Error Capture measurement mode.
<i>":<Handle>:SGENeral:GLOBal:CONFigure:CCAPture" on page 153</i>	Sets the instrument to Compare and CAPture mode.
<i>":FETCh[:ECOunt]?" on page 312</i>	Activates the Error Count measurement mode.
<i>":ECOunt:RESet" on page 315</i>	Resets the "received bit counter" and the "failed bit counter" to zero.
<i>":<Handle>:SGENeral:GLOBal:FETCh:ERRor:ANY?" on page 144</i>	Reports whether there has been found any error.
<i>":FETCh:ERRor:ANY?" on page 312</i>	Returns whether there has been found any error for the specified port or terminal.

Level Parameter Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":OUTPut:TVOLtage" on page 272</i>	Sets the external termination voltage.
<i>":OUTPut:TVOLtage?" on page 272</i>	Returns the current programmed value for the external termination voltage for the connectors of the specified port/terminal/connector.
<i>":VOLtage[:LEVel][:IMMEDIATE]:HIGH" on page 225</i>	Sets the high level of the pulse.
<i>":VOLtage[:LEVel][:IMMEDIATE]:HIGH?" on page 226</i>	Returns the high level value for the specified port/terminal/connector.
<i>":VOLtage[:LEVel][:IMMEDIATE]:LOW" on page 227</i>	Sets the low level of the pulse.
<i>":VOLtage[:LEVel][:IMMEDIATE]:LOW?" on page 228</i>	Returns the low level value for the specified port/terminal/connector.
<i>":VOLtage[:LEVel][:IMMEDIATE]:CAConfiguration:LOW" on page 229</i>	Sets the additional low level of the pulse when channel addition mode is active.

Command (Link to detailed description)	Description
<i>":VOLTage[:LEVel][:IMMEDIATE]:CAConfiguration:LOW?" on page 230</i>	Returns the additional low level value for the specified port/terminal/connector when channel addition mode is active.
<i>":VOLTage[:LEVel][:IMMEDIATE]:SEMode" on page 231</i>	Sets whether or not single-ended channel operation mode is used.
<i>":VOLTage[:LEVel][:IMMEDIATE]:SEMode?" on page 232</i>	Returns whether or not single-ended channel operation mode is used.
<i>":VOLTage[:LEVel][:IMMEDIATE]:SEMode:AVAILable?" on page 232</i>	Returns whether or not single-ended channel operation mode is available.
<i>":SENSe:VOLTage:RANGe" on page 233</i>	Selects the allowed input voltage range.
<i>":SENSe:VOLTage:RANGe?" on page 233</i>	Returns the allowed input voltage range.

Amplitude/Offset Correction Factor Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":CALibration[:VOLTage]:OCFactor" on page 235</i>	Sets the offset correction factor of the port, terminal, or connector.
<i>":CALibration[:VOLTage]:OCFactor?" on page 235</i>	Returns the offset correction factor of the port, terminal, or connector.
<i>":CALibration[:VOLTage]:ACFactor" on page 236</i>	Sets the amplitude correction factor of the port, terminal, or connector.
<i>":CALibration[:VOLTage]:ACFactor?" on page 236</i>	Returns the amplitude correction factor of the port, terminal, or connector.
<i>":CALibration[:VOLTage]:HOLD" on page 237</i>	Sets the correction factor locking of the port, terminal, or connector.
<i>":CALibration[:VOLTage]:HOLD?" on page 237</i>	Returns the correction factor locking of the port, terminal, or connector.

Timing Parameter Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":PULSe:DElay" on page 185</i>	Sets the time from the start of the period to the first edge of the pulse.
<i>":PULSe:DElay?" on page 186</i>	Returns the delay value for the specified port/terminal/connector.
<i>":PULSe:WIDTh" on page 191</i>	Sets the width (duration) of the pulse.
<i>":PULSe:WIDTh?" on page 191</i>	Returns the width value for the specified port/terminal/connector.
<i>":PULSe:DElay:CYCLes" on page 186</i>	Sets the delay in cycles, where one cycle corresponds to the actual period/frequency valid for the specified generator output connector.
<i>":PULSe:DElay:CYCLes?" on page 187</i>	Returns the number of delay cycles.
<i>":PULSe:DElay:TIME" on page 188</i>	Sets the delay in seconds.
<i>":PULSe:DElay:TIME?" on page 188</i>	Returns the delay.
<i>":PULSe:DCYCLe" on page 192</i>	Sets the duty cycle of a repetitive pulse waveform.
<i>":PULSe:DCYCLe?" on page 192</i>	Returns the duty cycle value for the specified port/terminal/connector.
<i>":PULSe:HOLD" on page 193</i>	Sets width or duty cycle to hold.
<i>":PULSe:HOLD?" on page 193</i>	Returns the hold parameter valid for the specified port/terminal/connector.
<i>":PULSe:TRANSition[:LEADing]" on page 194</i>	Sets the leading edge value for the specified port/terminal/connector.
<i>":PULSe:TRANSition[:LEADing]?" on page 195</i>	Returns the leading edge value for the specified port/terminal/connector.
<i>":PULSe:TRANSition:TRAILing" on page 195</i>	Sets the trailing edge value for the specified port/terminal/connector.
<i>":PULSe:TRANSition:TRAILing?" on page 196</i>	Returns the trailing edge value for the specified port/terminal/connector.
<i>":PULSe:TRANSition:CAConfiguration[:LEADing]" on page 197</i>	Sets the additional leading edge value for the specified port/terminal/connector, when channel addition mode is active.
<i>":PULSe:TRANSition:CAConfiguration[:LEADing]?" on page 198</i>	Returns the additional leading edge value for the specified port/terminal/connector, when channel addition mode is active.
<i>":PULSe:TRANSition:CAConfiguration:TRAILing" on page 199</i>	Sets the trailing edge value for the specified port/terminal/connector.
<i>":PULSe:TRANSition:CAConfiguration:TRAILing?" on page 200</i>	Returns the additional trailing edge value for the specified port/terminal/connector when channel addition mode is active.
<i>":MUX" on page 201</i>	SetS the frequency multiply factor for the specified port/terminal/connector.
<i>":MUX?" on page 201</i>	Returns the current frequency multiply factor (MUX factor) for the specified port/terminal/connector.

MUX Parameter Commands

The following table lists the commands for setting/getting MUX parameters.

Command (Link to detailed description)	Description
<i>":VOLTage:AMPLitude" on page 206</i>	Sets the amplitude of the multiplexer output signal.
<i>":VOLTage:AMPLitude?" on page 206</i>	Returns the amplitude of the multiplexer output signal.
<i>":VOLTage:OFFSet" on page 207</i>	Adds an offset voltage to the generated signal.
<i>":VOLTage:OFFSet?" on page 207</i>	Returns the amplitude of the offset voltage.
<i>":VOLTage:OFFSet:ENABle" on page 208</i>	Enables/disables voltage offset.
<i>":VOLTage:OFFSet:ENABle?" on page 208</i>	Returns the status of voltage offset.
<i>":OUTPut:EATTenuator" on page 209</i>	Sets the attenuation value of an external attenuator.
<i>":OUTPut:EATTenuator?" on page 209</i>	Returns the entered attenuation value of an external attenuator.
<i>":OUTPut:DELay:SWEEp" on page 210</i>	Sets the value for the additional delay.
<i>":OUTPut:DELay:SWEEp?" on page 211</i>	Returns the value for the additional delay.
<i>":OUTPut:DELay:SWEEp:MODE" on page 211</i>	Sets the delay correction or the delay calibration mode.
<i>":OUTPut:DELay:SWEEp:MODE?" on page 212</i>	Returns the current mode for the delay.
<i>":OUTPut:DELay:SWEEp:PRoM" on page 213</i>	The delay values of a MUX module are stored in the module's EEPROM. They are independent of the loaded setting. This command writes them to or reads them from the EEPROM.
<i>":TRIGger" on page 215</i>	Sets the source of the clock signal used for the timing of the E4868A multiplexer or E4869A demultiplexer.
<i>":TRIGger?" on page 215</i>	Returns the source of the clock signal used for the timing of the E4868A multiplexer or E4869A demultiplexer.
<i>":TRIGger:MODE" on page 216</i>	Sets the speed of the substrate clock output signal.
<i>":TRIGger:MODE?" on page 216</i>	Returns the speed of the substrate clock output signal.
<i>":INPut:THReshold" on page 251</i>	Specifies the threshold voltage of an input connector (only available for the E4969B).
<i>":INPut:THReshold?" on page 251</i>	Returns the current threshold voltage of the specified input connector (only available for the E4969B).

DeMUX Parameter Commands

The following table lists the commands for setting/getting DeMUX parameters.

Command (Link to detailed description)	Description
<i>":INPut:OCOMPensation" on page 214</i>	Sets the decision threshold for sampling the incoming signal.
<i>":INPut:OCOMPensation?" on page 214</i>	Returns the decision threshold for sampling the incoming signal.
<i>":TRIGger" on page 215</i>	Sets the source of the clock signal used for the timing of the E4868A multiplexer or E4869A demultiplexer.
<i>":TRIGger?" on page 215</i>	Returns the source of the clock signal used for the timing of the E4868A multiplexer or E4869A demultiplexer.
<i>":INPut:DElay:SWEEP" on page 259</i>	Sets the delay sweep value (only available for the E4969B).
<i>":INPut:DElay:SWEEP?" on page 259</i>	Returns the current delay sweep value (only available for the E4969B).
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:REWire" on page 219</i>	Switches the DeMUX rewiring on or off.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:REWire?" on page 219</i>	Returns the current state of the DeMUX rewiring.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RMODE" on page 220</i>	Sets the modes of DeMUX rewiring.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RMODE?" on page 221</i>	Returns the current mode of DeMUX rewiring.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RCH" on page 221</i>	Switches the rewire verify mode on and off.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RCH?" on page 222</i>	Returns the current rewire verify mode.
<i>":<Handle>:SGENeral:PDATA:DMUX:STAGe" on page 222</i>	Sets the number of stages of the demultiplexer.
<i>":<Handle>:SGENeral:PDATA:DMUX:STAGe?" on page 223</i>	Returns the number of stages of the demultiplexer.
<i>":<Handle>:SGENeral:PDATA:DMUX:STAGe:OUT" on page 223</i>	Sets the number of outputs per demultiplexer for a specified stage.
<i>":<Handle>:SGENeral:PDATA:DMUX:STAGe:OUT?" on page 224</i>	Returns the number of outputs per demultiplexer for a specified stage.

DeMUX Rewiring Commands

The following table lists the DeMUX rewiring commands.

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:REWire" on page 219</i>	Switches the DeMUX rewiring on or off.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:REWire?" on page 219</i>	Returns the current state of the DeMUX rewiring.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RMODE" on page 220</i>	Sets the modes of DeMUX rewiring.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RMODE?" on page 221</i>	Returns the current mode of DeMUX rewiring.

Command (Link to detailed description)	Description
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RCH" on page 221</i>	Switches the rewire verify mode on and off.
<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RCH?" on page 222</i>	Returns the current rewire verify mode.
<i>":<Handle>:SGENeral:PDATa:DMUX:STAGe" on page 222</i>	Sets the number of stages of the demultiplexer.
<i>":<Handle>:SGENeral:PDATa:DMUX:STAGe?" on page 223</i>	Returns the number of stages of the demultiplexer.
<i>":<Handle>:SGENeral:PDATa:DMUX:STAGe:OUT" on page 223</i>	Sets the number of outputs per demultiplexer for a specified stage.
<i>":<Handle>:SGENeral:PDATa:DMUX:STAGe:OUT?" on page 224</i>	Returns the number of outputs per demultiplexer for a specified stage.

Delay Control Parameter Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":DCONtrol[:DEViation]?" on page 239</i>	Returns the current maximum delay control deviation in seconds.
<i>":DCONtrol:SENSitivity" on page 240</i>	Sets the delay control sensitivity of the external delay control modulation signal.
<i>":DCONtrol:SENSitivity?" on page 240</i>	Returns the delay control sensitivity of the external delay control modulation signal.
<i>":DCONtrol:SOURce" on page 241</i>	Sets the delay control source.
<i>":DCONtrol:SOURce?" on page 242</i>	Returns the delay control source.
<i>":DCONtrol:STATe" on page 243</i>	Switches the specified external delay control input connector on or off.
<i>":DCONtrol:STATe?" on page 244</i>	Returns the current state of the specified external delay control input connector.

Input Parameter Commands

The following table lists the commands available for data ports only. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":INPut[:STATe]" on page 245</i>	Enables or disables an analyzer input connector.
<i>":INPut[:STATe]?" on page 245</i>	Returns the current status of the specified analyzer input connector.
<i>":INPut:TVOLtage" on page 250</i>	Specifies the termination voltage of an analyzer input connector.
<i>":INPut:TVOLtage?" on page 250</i>	Returns the current termination voltage of the specified analyzer input connector.
<i>":INPut:THReshold" on page 251</i>	Specifies the threshold voltage of an analyzer input connector.
<i>":INPut:THReshold?" on page 251</i>	Returns the current threshold voltage of the specified analyzer input connector.

Command (Link to detailed description)	Description
<i>":INPut:DElay" on page 255</i>	Specifies the delay of the sampling edge.
<i>":INPut:DElay?" on page 255</i>	Returns the current delay of the sampling edge for the specified analyzer input connector.
<i>":INPut:DElay:CYCLes" on page 256</i>	Specifies the delay of the sampling edge in terms of cycles corresponding to the actual period/frequency valid for the specified analyzer input connector.
<i>":INPut:DElay:CYCLes?" on page 256</i>	Returns the current delay of the sampling edge for the specified analyzer input connector in terms of cycles.
<i>":INPut:DElay:TIME" on page 257</i>	Specifies the delay of the sampling edge.
<i>":INPut:DElay:TIME?" on page 257</i>	Returns the current delay of the sampling edge for the specified analyzer input connector.
<i>":INPut:DElay:ACTual?" on page 258</i>	Returns the actual delay after synchronization.
<i>":INPut:DElay:SWEEp" on page 259</i>	Sets the delay sweep value.
<i>":INPut:DElay:SWEEp?" on page 259</i>	Returns the current delay sweep value.
<i>":INPut:POLarity" on page 246</i>	Sets the input polarity of the specified data port/terminal/connector to either normal or inverted.
<i>":INPut:POLarity?" on page 246</i>	Returns the input polarity of the specified port/terminal/connector.
<i>":INPut:TYPE" on page 247</i>	Selects how the E4835A, E4863A, and E4865A differential input frontends are sampled.
<i>":INPut:TYPE?" on page 248</i>	Returns the operation mode of the E4835A, E4863A, and E4865A differential input frontend.
<i>":INPut:MODE" on page 248</i>	Selects between single-ended termination and differential termination mode.
<i>":INPut:MODE?" on page 249</i>	Returns the termination mode of an input frontend.
<i>":SENSe:VOLTag:e:RANGe" on page 233</i>	Selects the allowed input voltage range for the E4835A differential input frontend.
<i>":SENSe:VOLTag:e:RANGe?" on page 233</i>	Returns the currently selected input voltage range of an E4835A differential input frontend.
<i>":INPut:IMPedance[:INTernal]" on page 252</i>	Specifies the internal termination impedance of the analyzer input connector.
<i>":INPut:IMPedance[:INTernal]?" on page 252</i>	Returns the current internal impedance of the specified analyzer input connector.
<i>":INPut:SEQuence[:LAYer:SOURce:]CLOCK" on page 252</i>	Sets the clock source mode for a module.
<i>":INPut:SEQuence[:LAYer:SOURce:]CLOCK?" on page 253</i>	Returns the currently used clock source mode for a module.
<i>":INPut:SERial" on page 254</i>	Specifies a serial impedance on this analyzer input connector.
<i>":INPut:SERial?" on page 254</i>	Returns the current serial impedance used for the specified analyzer input connector.

Command (Link to detailed description)	Description
<i>":INPut:TCONfig" on page 260</i>	Selects the termination model for input frontends.
<i>":INPut:TCONfig?" on page 261</i>	Returns the termination model for input frontends.
<i>":INPut:DIMPedance" on page 261</i>	Sets the impedance between the IN and \IN\ inputs of an E4835A, E4863A and E4865A frontend when the differential termination model is selected.
<i>":INPut:DIMPedance?" on page 262</i>	Returns the differential termination resistor.
<i>":INPut:DISConnect:MODE?" on page 262</i>	Returns how the specified connector is to be disconnected when the <code>SGENeral:GLOBal:CONNect OFF</code> command is executed.
<i>":INPut:DISConnect:MODE" on page 263</i>	Sets how the specified connector is to be disconnected when the <code>SGENeral:GLOBal:CONNect OFF</code> command is executed.

Optical Input Commands

The following table lists the commands available for data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":INPut:OPTic[:STATe][:VALue]" on page 264</i>	Sets the state of the optical channel(s).
<i>":INPut:OPTic[:STATe][:VALue]?" on page 264</i>	Queries the state of the optical channel(s).
<i>":INPut:OPTic:POWer:UNIT[:VALue]" on page 265</i>	Sets the unit for the 0/1 decision threshold of the selected optical input connector, port, or terminal.
<i>":INPut:OPTic:POWer:UNIT[:VALue]?" on page 265</i>	Queries the unit for the 0/1 decision threshold of the selected optical input connector, port, or terminal.
<i>":INPut:OPTic:POWer:THReshold[:VALue]" on page 266</i>	Sets the 0/1 decision threshold of the selected optical input connector, port, or terminal.
<i>":INPut:OPTic:POWer:THReshold[:VALue]?" on page 266</i>	Queries the 0/1 decision threshold of the selected optical input connector, port, or terminal.
<i>":INPut:OPTic:WAVelength[:VALue]" on page 266</i>	Sets the standard calibration wavelength.
<i>":INPut:OPTic:WAVelength[:VALue]?" on page 267</i>	Returns the standard calibration wavelength.
<i>":INPut:OPTic:MEASure" on page 267</i>	Measures the average signal power and sets this as the 0/1 decision threshold on the selected optical input connector, port, or terminal.
<i>":INPut:OPTic:DLCalibration" on page 267</i>	Performs dark level calibration on the selected optical input connector, port, or terminal.

Output Parameter Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":OUTPut[:STATe]" on page 268</i>	Controls whether the connectors of the specified port/terminal/connector are opened or closed.
<i>":OUTPut[:STATe]?" on page 269</i>	Returns the current connection state for the connectors of the specified port/terminal/connector.
<i>":OUTPut:CStAtE" on page 271</i>	Controls whether the complement connectors of the specified port/terminal/connector are opened or closed.
<i>":OUTPut:CStAtE?" on page 271</i>	Returns the current connection state for the complement connectors of the specified port/terminal/connector.
<i>":OUTPut:TVOLtAge" on page 272</i>	Sets the external termination voltage.
<i>":OUTPut:TVOLtAge?" on page 272</i>	Returns the current programmed value for the external termination voltage for the connectors of the specified port/terminal/connector.
<i>":OUTPut:POLarity" on page 270</i>	Sets the output polarity of the specified data port/terminal/connector to either normal or inverted.
<i>":OUTPut:POLarity?" on page 270</i>	Returns the output polarity of the specified port/terminal/connector.
<i>":OUTPut:IMPedance:EXTernal" on page 273</i>	Sets the external termination impedance, the real load impedance of the DUT.
<i>":OUTPut:IMPedance:EXTernal?" on page 273</i>	Returns the currently set value for the termination (load) impedance.
<i>":OUTPut:TCONfig" on page 274</i>	Selects the termination model for output frontends.
<i>":OUTPut:TCONfig?" on page 275</i>	Returns the termination model for output frontends.
<i>":OUTPut:DIMPedance:EXTernal" on page 276</i>	Sets the impedance between the OUT and \OUT\ outputs of an E4838A or E4843A frontend when the differential termination model is selected.
<i>":OUTPut:DIMPedance:EXTernal?" on page 276</i>	Returns the differential termination impedance.
<i>":OUTPut:CAConfiguration[:MODE]" on page 277</i>	Selects the channel-add mode of a port/terminal/ connector.
<i>":OUTPut:CAConfiguration[:MODE]?" on page 278</i>	Returns the current channel addition mode of the specified port/terminal/connector.
<i>":OUTPut:DISConnect:MODE?" on page 278</i>	Returns how the specified connector is to be disconnected when the SGENeral:GLOBal:CONNect OFF command is executed.
<i>":OUTPut:DISConnect:MODE" on page 279</i>	Sets how the specified connector is to be disconnected when the SGENeral:GLOBal:CONNect OFF command is executed.

Optical Output Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":OUTPut:OPTic:STATe[:VALue]" on page 281</i>	Enables/disables the laser on the E/O converter.
<i>":OUTPut:OPTic:STATe[:VALue]?" on page 282</i>	Queries the state of the laser on the E/O converter.
<i>":OUTPut:OPTic:METhod[:VALue]" on page 283</i>	Defines the method used for setting optical power values.
<i>":OUTPut:OPTic:METhod[:VALue]?" on page 283</i>	Queries the currently used method for setting optical power values.
<i>":OUTPut:OPTic:POWer:UNIT[:VALue]" on page 284</i>	Sets the unit for all power parameters of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:UNIT[:VALue]?" on page 284</i>	Queries the unit for all power parameters of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:AVERAge[:VALue]" on page 285</i>	Sets the average power of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:AVERAge[:VALue]?" on page 285</i>	Queries the average power of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:MAmplitude[:VALue]" on page 286</i>	Sets the modulation of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:MAmplitude[:VALue]?" on page 287</i>	Queries the modulation amplitude of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:HIGH[:VALue]" on page 287</i>	Sets the high power of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:HIGH[:VALue]?" on page 288</i>	Queries the high power of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:LOW[:VALue]" on page 288</i>	Sets the low power of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:POWer:LOW[:VALue]?" on page 289</i>	Queries the low power of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:ERATio[:VALue]" on page 289</i>	Sets the extinction ratio of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:ERATio[:VALue]?" on page 290</i>	Queries the extinction ratio of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:ERATio:UNIT[:VALue]" on page 290</i>	Sets the unit used for the extinction ratio of the selected optical output connector, port, or terminal.
<i>":OUTPut:OPTic:ERATio:UNIT[:VALue]?" on page 291</i>	Queries the unit used for the extinction ratio of the selected optical output connector, port, or terminal.

Clock Trigger Output Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:HIGH" on page 292</i>	Sets the high level for the trigger output of the clock module.
<i>":CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:HIGH?" on page 292</i>	Returns the high level for the trigger output of the clock module.
<i>":CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:LOW" on page 293</i>	Sets the low level for the trigger output of the clock module.
<i>":CLOCK[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]:LOW?" on page 293</i>	Returns the low level for the trigger output of the clock module.
<i>":CLOCK[:SOURce]:PULSe:DELay:SWEEP" on page 293</i>	Sets the delay of the trigger output of the clock module.
<i>":CLOCK[:SOURce]:PULSe:DELay:SWEEP?" on page 294</i>	Returns the delay of the trigger output of the clock module.
<i>":CLOCK:OUTPut:IMPedance:EXternal" on page 294</i>	Sets the external impedance of the trigger output of the clock module.
<i>":CLOCK:OUTPut:IMPedance:EXternal?" on page 294</i>	Returns the external impedance of the trigger output of the clock module.
<i>":CLOCK:OUTPut:DIMPedance:EXternal" on page 295</i>	Sets the external differential impedance of the trigger output of the clock module.
<i>":CLOCK:OUTPut:DIMPedance:EXternal?" on page 295</i>	Returns the external differential impedance of the trigger output of the clock module.
<i>":CLOCK:OUTPut:TCONfig" on page 296</i>	Sets the differential termination resistance of the trigger output of the clock module.
<i>":CLOCK:OUTPut:TCONfig?" on page 297</i>	Returns the differential termination resistance of the trigger output of the clock module.
<i>":CLOCK:OUTPut:TVOLTage" on page 297</i>	Sets the external termination voltage of the trigger output of the clock module.
<i>":CLOCK:OUTPut:TVOLTage?" on page 298</i>	Returns the external termination voltage of the trigger output of the clock module.

Auxiliary Out Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":AOUT[:MONitor]" on page 298</i>	Sets the signal at the AUX output of a N4873A/75A module.
<i>":AOUT[:MONitor]?" on page 299</i>	Gets the signal at the AUX output of a N4873A/75A module.

Performance Parameter Commands


The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":SIGNal:MODE"</i> on page 316	Sets the performance mode for the clock signal (not available for all clock modules).
<i>":SIGNal:MODE?"</i> on page 317	Returns the performance mode for the clock signal (not available for all clock modules).

Format Parameter Commands

The following table lists the commands available for pulse and data ports. The commands are available at port, terminal, and connector level.

Command (Link to detailed description)	Description
<i>":FORMat"</i> on page 318	Controls the output connectors data format of the specified port/terminal/connector.
<i>":FORMat?"</i> on page 319	Returns the current data format state for the output connectors of the specified port/terminal/connector.



Commands in the DVT Subsystem

The DVT subsystem is always available. The commands in this subsystem provide basic administration features.

This reference starts with an introductory example and then lists the available commands and subsystems:

- DVT
 - Top-level command :DVT:IDN?
 - :SYSTem Subsystem
 - :INSTrument Subsystem
 - :INSTrument:HANDle Subsystem
 - :MMEMory Subsystem

Example: Use of :DVT Subsystem Commands

```
:DVT:INST:LIST?                # check for instrument types
                                # available
                                # Returns: "DSR"

:DVT:INST:RES:LIST? "DSR"      # check for available virtual
                                # instruments
                                # Returns: "DSR1"

                                # query to get a handle for the
                                # virtual instrument. _TEST is a
                                # suggestion:
:DVT:INST:HAND:CRE? _TEST, "DSR", "DSR1"
                                # The suggested handle is accepted.
                                # Returns: _TEST

:DVT:INST:HAND:LIST?           # Lists the handles in use
                                # Returns: "DVT", "_TEST"

:_TEST:IDN?                    # Queries for the virtual instrument
                                # identification
                                # Returns:
                                # Agilent Technologies,E4875A,0,0

:DVT:instrument:handle:destroy _TEST
                                # destroy the handle _TEST
                                # (do not forget the underscore)
```

Top-Level Commands

On top level of the DVT subsystem there is only one command available:

- `:DVT:IDN?`

:DVT:IDN?

Command `:DVT:IDN?`

Syntax `:DVT:IDN?`

Description Identifies the device.

The response consists of the following four fields (fields are separated by commas):

- Manufacturer
- Model Number
- Serial Number (returns 0 if not available)
- Firmware Revision (returns 0 if not available)

Example `:dvt:idn?`

might return

```
Agilent Technologies,Agilent 81200, 0, 0
```

:SYSTem Subsystem

The DVT:SYSTem subsystem supports the following command:

- :DVT:SYSTem:ERRor?

:DVT:SYSTem:ERRor?

Command :DVT:SYSTem:ERRor?

Syntax :DVT:SYSTem:ERRor?

Description The query returns the first entry of the error queue and removes it from the queue. As long as the command does not return 0, "No error", there are further errors in the queue.

Example :dvt:syst:err?

might return

0, "No error"

:INSTRUMENT Subsystem

The :INSTRUMENT subsystem provides a mechanism to identify available applications and create handles for virtual instruments (see *"The Command Tree" on page 32*).

The :DVT:INSTRUMENT subsystem supports the following commands:

- DVT:INSTRUMENT
 - :LIST?
 - :RESOURCE:LIST?
 - :HANDLE Subsystem

:DVT:INSTRUMENT:LIST?

Syntax :DVT:INSTRUMENT:LIST?

Description The LIST? query returns a comma-separated list of <character response data> items containing the names of all applications.

Example :DVT:INST:LIST?
might return
"DSR"

:DVT:INSTRUMENT:RESOURCE:LIST?

Syntax :DVT:INSTRUMENT:RESOURCE:LIST? <"Application">

Parameters <quoted string> The name of the desired application
The response is a comma-separated list of <character response data> items.

Description The LIST? query returns a comma-separated list of hardware resources which may be connected to the specified application.

Example :DVT:INSTRUMENT:RESOURCE:LIST? "DSR"
might return
"DSRA"

:INSTrument:HANDle Subsystem

Syntax :DVT:INSTrument:HANDle

The HANDle subsystem collects the functions that are related to virtual instrument management.

:DVT:INSTrument:HANDle:CREate?

Syntax :DVT:INSTrument:HANDle:CREate? <Handle>, <"Application">, <"Resource">

Parameters <Handle> Suggested value for the Handle

<"Application"> The name of the desired application. The available applications may be listed using :DVT:INST:LIST?.

<"Resource"> The name of the hardware resource with which the new virtual instrument should be associated. Available resources may be listed using :DVT:INST:RES:LIST?.

Description Creates a new virtual instrument.

Return A <Character Response Data> element containing the name of the new handle is returned. <Handle> will be used if possible. If <Handle> is illegal for any reason, a legal and unique handle will be generated and returned.

A valid handle always starts with a "_" (it must match the following regular expression: `_[a-zA-Z0-9]*[a-zA-Z]`).

Example :DVT:INST:HAND:CRE? _TEST, "DSR", "DSR1"

:DVT:INST:HAND:CRE? TEST, "DSR", "DSR1"

might return

_TEST

:DVT:INSTrument:HANDle:LIST?

Syntax :DVT:INSTrument:HANDle:LIST?

Returns a comma-separated list of all virtual instrument handles. The list will always contain the handle DVT.

Example DVT:INST:HAND:LIST?
might return "DVT", "_TEST"

:DVT:INSTrument:HANDle:DESTroy

Syntax DVT:INSTrument:HANDle:DESTroy <Handle>

Parameters <Handle> The handle of the virtual instrument to be destroyed.
Destroys a handle created by CREate? and frees all associated resources.

Example DVT:INST:HAND:DEST _TEST

:MMEMory Subsystem

The DVT:MMEMory subsystem supports the following commands:

- :DVT:MMEMory
 - :SETTing:EXPort
 - :SETTing:EXPort?
 - :SETTing:IMPort:DVT:MMEMory:SETTing:EXPort

Syntax :DVT:MMEMory:SETTing:EXPort <Handle>,
<"FileName">[,<YDELay | NDELay | ODELay>]

Parameters <Handle> The handle of the virtual instrument.

<"FileName"> The name of the file that will be created.

YDELay Yes delay; export setting with cable delay parameters.

NDELay No delay; export setting without cable delay parameters.

ODELay Only delay; export only cable delay parameters.

Description The system generates a file with the described setting. The optional parameter filters the cable delay parameters.

Example :DVT:MMEM:SETT:EXP _TEST, "c:\ParBERT_Exchange\withdel.txt", YDEL

:DVT:MMEMory:SETTing:EXPort?

Syntax :DVT:MMEMory:SETTing:EXPort? <Handle> [,<YDELay | NDELay | ODELay>]

Parameters <Handle> The handle of the virtual instrument.

YDELay Yes delay; export setting with cable delay parameters.

NDELay No delay; export setting without cable delay parameters.

ODELay Only delay; export only cable delay parameters.

Description The query returns an expression describing the current setting. The optional parameter filters the cable delay parameters.

Example :DVT:MMEM:SETT:EXP? _TEST, NDEL

:DVT:MMEMory:SETTing:IMPort

Syntax :DVT:MMEMory:SETTing:IMPort <Handle>,
<"Filename">|<(Expression)>

Parameters **<Handle>** The handle of the virtual instrument for which the setting is supposed to be used.


<"Filename"> The name of a file that contains a series of SCPI commands describing the setting.

<Expression> A set of commands in form of an expression. The commands have to be listed without the <Handle> subnode.

TIP Use the :DVT:MMEMory:SETTing:EXPort? command to see the necessary format.

Description This command makes it possible to import a setting into the Agilent 81250 System.

Example :DVT:MMEM:SETT:IMP _TEST, "c:\ParBERT_Exchange\setting1.txt"



Commands in DSR Application Subsystems

This chapter describes the commands available for the DSR application of the Agilent 81250 system. The general commands always available for the system are described in *“Commands in the DVT Subsystem” on page 67*.

For basic information on the command syntax and the command tree, please refer to *“Overview of the SCPI Command Structure” on page 29*.

Each command and query entry has at least some of the following items:

- Full command syntax
- Brief description
- Parameters
- Return value
- Possible error conditions
- Cross-references to related commands
- Short example showing context in which the command is used, its effect and return value

Administration Commands

On top level, there are commands for managing the system.

:<Handle>:IDN?

Syntax :<Handle>:IDN?

Description Identifies the device.

The response consists of the following four fields (fields are separated by commas):

- Manufacturer
- Model Number
- Serial Number (returns 0 if not available)
- Firmware Revision (returns 0 if not available)

Example :_test:IDN?

might return:

```
Agilent Technologies,E4875A,0,Rev. 1.01
```

:<Handle>:OPC?

Syntax :<Handle>:OPC?

Return Value The query returns when all modules report that they are ready.

Data is not available at the outputs immediately after an SGEN:GLOB:INIT:CONT ON command is sent, because of the pipelined system architecture.

Returns 1 when all pending operations are finished.

Example :_test:SGEN:GLOB:PER 100e-9

```
:_test:OPC?
```

:SYSTem Subsystem

Syntax :<Handle>:SYSTem

The :SYSTem subsystem provides commands to check errors or to switch on/off the internal error check system.

:<Handle>:SYSTem:ERRor?

Syntax :<Handle>:SYSTem:ERRor?

Return Value When errors are detected, they are placed in a queue. This command returns the first entry of the error queue to the user.

Example :_test:SYST:ERR?

might return for example:

0, "No error"

or, another example:

-300, "Device-specific error; 2001 Terminal suffix out of range"

:<Handle>:SYSTem:CINFormation?

Syntax	:<Handle>:SYSTem:CINFormation? <SHORT DETailed> [,<FileName>]
Parameters	<“FileName”> (Optional) The settings file for the system.
Description	This query returns the system configuration information. For each element, the subelements are listed (for example, for a mainframe, the modules in that mainframe are listed; for each module, the frontends are listed).
Return Value	The response is an expression with the description of all elements in the following syntax: <ul style="list-style-type: none"> <ModuleInfo> ::= (“<ProductNr> “,” <SpeedClass> [“,” <SerNr> “,” <IDNr>] “,” <ConnInfo> (“,” <ConnInfo>)* “” <ConnInfo> ::= (“<ProductNr> “,” <SpeedClass> “,” “Type” [“,” <SerNr> “,” <IDNr> “,” <ConnNr>] “” <ProductNr> ::= for example, “E4838A” <SpeedClass> ::= for example, 660 <Type> ::= “ANALYZER” “GENERATOR” <SerNr> ::= serial number (0 if not available) <IDNr> ::= identification number (0 if not available) <ConnNr> ::= “S1” “D1” “D2” <ul style="list-style-type: none"> S1: single frontend D1: first connector of a dual frontend D2: second connector of a dual frontend

The optional syntax elements only appear if DETailed is selected.

Example :_test:SYST:CINF? SHOR
could return, for example (reformatted only for readability):

```
((E4805B,660),
(E4861A,2640,
(E4863A,2640,ANALYZER),
(E4862A,2640,GENERATOR)),
(E4861A,2640,
(E4863A,2640,ANALYZER),
(E4862A,2640,GENERATOR)))
```

:<Handle>:SYSTem:TEST:MODule

Syntax :<Handle>:SYSTem:TEST:MODule DETailed | SHORt [,CGR#, MOD#]

Description A module selftest is started by the firmware on every module. The results of this test are stored in the message queue. The message queue can be read by with the command :SYST:MQU?.

Parameters The format of the messages can be specified by following keywords:

<DETailed> Generates a more detailed message.

<SHORt> Generates a less detailed message.

[,CGR#, MOD#] A single module can be specified by the optional parameters. The first parameter (CGR#) is the clock group the module belongs to, the second parameter (MOD#) is the number of the module itself.

Example For a SHORt message:

```
(1,3,1,4,'E4861A','Passed','E4861A Ver: 1.92 E4863 E4862 ','No error')
```

For a DETailed message:

```
= (1,1,1,2,'E4805B','Failed','< AGILENT TECHNOLOGIES, E4805B, 01, <>, "", Module Software Version = 1.81, Boot Loader Version = 1.00 >','-330, Self-test failed: Frequency generation PLL test failed: high limit not reached!-330, Self-test failed: Frequency generation PLL test failed: high limit not reached!')
```

A DETailed message for an E4861A could appear as:

```
(1,4,1,7,'E4861A','Failed','< AGILENT TECHNOLOGIES, E4861A, 00, <>, "", Module Software Version = 0.32, Boot Loader Version = 0.01, <E4863, 01, <>, ">, <E4862, 01, <>, "> >','-330, Self-test failed: Voltage of +5VRef is out of valid range')
```

:<Handle>:SYSTem:TEST:GLOBal

- Syntax** :<Handle>:SYSTem:TEST:GLOBal DETailed | SHORt
- Description** This command initiates a system-wide selftest. The local bus and the SYSClk signal distribution is tested. The selftest messages are placed in the message queue. First the message queue is cleared, and then the new results will be inserted.
- Parameters** The format of the messages can be specified by following keywords:
- <DETailed> Generates a more detailed message.
 - <SHORt> Generates a less detailed message.

:<Handle>:MODule:SREVisions

- Syntax** :<Handle>:MODule:SREVisions DETailed | SHORt
- Description** This command checks the actual BIOS Software REVisions against the expected revision located in the firmware. The results of this test are located in the message queue.
- The message queue can be read with the command :SYST:MQU?
- Parameters** The format of the messages can be specified by following keywords:
- <DETailed> Generates a more detailed message.
 - <SHORt> Generates a less detailed message.
- Return Values** The following values may be placed in the message queue:
- BIOS: Update is needed
 - BIOS: Update is not needed
- The module selftest message is replaced by the expected revision.

:<Handle>:SYSTem:MQUeue[:READ]?

Syntax :<Handle>:SYSTem:MQUeue[:READ]?

Return Value Returns and then deletes the first item contained in the message queue. The next execution of this command reports the next message contained in the queue.

If the queue is empty, “()” is returned.

This command can be used, for example, to read the message queue after selftests have been executed for all modules. It has to be executed for each module.

NOTE The :READ option has no effect.

:<Handle>:SYSTem:MQUeue:LENGth?

Syntax :<Handle>:SYSTem:MQUeue:LENGth?

Return Value Returns the number of messages in the message queue.

:<Handle>:SYSTem:PON[:STATus]

Syntax :<Handle>:SYSTem:PON[:STATus] DETailed | SHORt

Description Moves the messages that are generated by the modules at system start up into the message queue. This command does *not* start a new selftest.

The message queue can be read with the command :SYST:MQU?.

Parameters A DETailed message is required for service purposes (in-depth message according to the Service selection on the GUI), SHORt is a summary status according to the user selection in the GUI.

:SYSTem:CLient Subsystem

Syntax :<Handle>:SYSTem:CLient

More than one client can simultaneously operate with the firmware server (for example, GUI-client, GPIB-client, VEE-client, ...).

To avoid conflicts, the commands in this subsystem control the firmware access. These commands allow using a system (virtual instrument) exclusively. There are two locking commands, which differ in the reaction of the locked application:

- If a system is locked by a client using the LOCK command, any access by another client returns an error code.
- If a system is locked by a client using the BLOCK command, any access by another client will simply wait until the system is unlocked, thus blocking the client. No error code is returned.

:<Handle>:SYSTem:CLient[:HANDLE]?

Syntax :<Handle>:SYSTem:CLient[:HANDLE]?

Return Value This query returns the name of the client that has currently locked the server. An empty string is returned if the server is not locked.

Example :_test:SYST:CLI?

might return for example:

_GPIB

:<Handle>:SYSTem:CLient:LOCK

Syntax :<Handle>:SYSTem:CLient:LOCK

This command can be used to take over the control of the virtual instrument explicitly.

If another client tries to access a locked virtual instrument, the error code -19, "ANOTHER_CLIENT_USES_APPLICATION" is returned.

NOTE A locked virtual instrument can be blocked by calling:
SYSTem:CLient:BLOCK.

Example :_test:SYST:CLI:LOCK

:<Handle>:SYSTem:CLient:BLOCK

Syntax :<Handle>:SYSTem:CLient:BLOCK

Description This command is used to take over the control of the virtual instrument explicitly.

If another client sends a command to a blocked virtual instrument, the command does not return until the instrument is unlocked (thus blocking the sender). No error message is returned.

The usage of this command should be restricted to *short* accesses.

NOTE A blocked virtual instrument can only be locked by calling: SYSTem:CLient:LOCK.

Example :_test:SYST:CLI:BLOCK

:<Handle>:SYSTem:CLient:UNLOCK

Syntax :<Handle>:SYSTem:CLient:UNLOCK

Description This command is used to unlock (or "free") the virtual instrument. This command performs an undo of SYSTem:CLient:LOCK and SYSTem:CLient:BLOCK.

Example :_test:SYST:CLI:UNLOCK

:CONFiguration Subsystem

Syntax :<Handle>:CONFiguration

:<Handle>:CONFiguration:CGROUPS(*)?

Syntax :<Handle>:CONFiguration:CGROUPS(*)?

Return Value Returns the number of available clock groups. The (*) specifier is ignored.

Related Commands *“[:CGROUP(*)] Subsystem” on page 123*

Example :_test:CONF:CGR?

might return:

1

:<Handle>:CONFiguration:CGROUPS(*):MODULES(*)?

Syntax :<Handle>:CONFiguration:CGROUPS(*):MODULES(*)?

Return Value Returns the number of modules contained in the specified clock group. The (*) specifier for modules is ignored.

Related Commands *“[:CGROUP(*)] Subsystem” on page 123*

Example :_test:CONF:CGR1:MOD?

might return:

3

:<Handle>:CONFiguration:CGROUPS(*): MODULES(*):CONNECTORS(*)?

Syntax :<Handle>:CONFiguration:CGROUPS(*):MODULES(*):CONNECTORS(*)?

Return Value Returns the number of connectors of the specified module. The (*) specifier for connectors is ignored.

Related Commands “[:CGROUP(*)] Subsystem” on page 123

Example :_test:CONF:CGR1:MOD2:CONN?
might return:
4

:<Handle>:CONFiguration:CGROUPS(*): MODULES(*):CONNECTORS(*):TYPE?

Syntax :<Handle>:CONFiguration:CGROUPS(*):MODULES(*):CONNECTORS(*):TYPE?

Return Value Returns the type of the specified connector.

Related Commands “[:CGROUP(*)] Subsystem” on page 123

Example :_test:CONF:CGR1:MOD2:CONN1:TYPE?
might return:
ANALYZER

:<Handle>:CONFiguration:STYPES?

Syntax :<Handle>:CONFiguration:STYPES?

Return Value Returns a list of scheme types supported by the Agilent 81250 System. See also “:SGENERAL Subsystem” on page 140.

Example :_test:CONF:STYP?
might return:
"SCHEME_GENERAL"

:<Handle>:CONFiguration:PROFile[:VALue]

- Syntax** :<Handle>:CONFiguration:PROFile[:VALue] <"ParameterName">, <(Expression)>
- Parameters** <"ParameterName"> Name of parameter to be set.
<(Expression)> Specified value.
- Description** Sets the parameter <"ParameterName"> to <(Expression)>.
- Return Value** None
- Example** :_test:CONF:PROF "PARAM1", (10d,10,"TEXT",10u,10f)

:<Handle>:CONFiguration:PROFile[:VALue]?

- Syntax** :<Handle>:CONFiguration:PROFile[:VALue]? <"ParameterName">
- Parameters** <"ParameterName"> Name of parameter to be queried.
- Return Value** Returns the value of <"ParameterName">.
- Example** :_test:CONF:PROF? "PARAM1"
might return:
(10d,10,"TEXT",10u,10f)

:<Handle>:CONFiguration:PROFile:REMOve

- Syntax** :<Handle>:CONFiguration:PROFile:REMOve <"ParameterName">
- Parameters** <"ParameterName"> Parameter Name
Removes the specified parameter contained in the "profile".
- Return Value** None
- Example** :_test:CONF:PROF:REM "PARAM1"

:<Handle>:CONFiguration:PROFile:LIST?

Syntax :<Handle>:CONFiguration:PROFile:LIST?

Description Lists the parameters contained in the “profile”.

Return Value None

Example :_test:CONF:PROF:LIST?

might return:

"PARAM1 "

:MMEMory Subsystem

Syntax :<Handle>:MMEMory

The :MMEMory subsystem provides mass storage capabilities. The mass storage may be either an internal or external drive, e.g.: hard disc drive, floppy disc drive, etc.

:<Handle>:MMEMory:LIST?

Syntax :<Handle>:MMEMory:LIST? <"Absolute Path">

Parameters <"Absolute Path"> Path of directory to be checked using "/" as path separator.

Return Value Returns a comma-separated list of the files in the specified directory.

If <"Absolute Path"> is an empty string, the root is listed. On Windows NT, the root is a virtual point below the drives. In other words, all drives are listed.

If <"Absolute Path"> does not point to a valid directory, an error is returned and the response is empty.

Example :_test:MMEM:LIST? "C:/"

Returns a list of the root directory of drive 'C':

```
("file_a", "file_b", "file_c", "file_d")
```

:<Handle>:MMEMory:INFormation?

Syntax :<Handle>:MMEMory:INFormation? <"Absolute Path">

Parameters <"Absolute Path"> Path of file object to be checked using "/" as path separator.

Return Value Returns detailed information about the specified file object. The response consist of an expression containing 5 comma-separated values like: <object type>, <mtime>, <size>, <attribute>, <db class>

<object type>	type of the object (quoted string)
<mtime>	modification time (numerical value)
<size>	size of object in bytes (numerical value)
<attributes>	attributes of the object (quoted string)
<db class>	type of a database object e.g. Setting, Segment, etc. (quoted string)

Returns the object type of drive 'C:'. "" (empty string) or 0 means not applicable.

Example :_test:MMEM:INF? "C:"

might return:

```
("DRIVE", 0, 0, "", "")
```

:<Handle>:MMEMory:SEGMent:LOAD

- Syntax** :<Handle>:MMEMory:SEGMent:LOAD
<"FileName">|<(Expression)>[,ON|OFF][,<"SettingName">]
- Parameters** First parameter
- <"FileName"> or <(Expression)>** Either specifies a file name containing segments or creates the segments according to the segment import and export syntax for loading it into the Agilent 81250 System's database (see "*Segment Import and Export Language*" on page 321).
- Optional second parameter
- [ON or OFF]** ON is the default. It means that if the specified file already exists, it will be overwritten (replaced) with the new segment properties and data pattern.
- Optional third parameter
- [<"SettingName">]** If a setting name is specified, the new or updated segments will be added as local segments to the specified setting. If the setting name is omitted, then the segments are placed in the global segment pool.
- Description** The command is used to import new or updated segments into the Agilent 81250 System's database.
- Return Value** None
- Example** :_test:MMEM:SEGM:LOAD "A:\TRAFFIC.txt", OFF, "TEST1"

:<Handle>:MMEMory:SEGMent:SAVE

Syntax Syntax 1:

```
:<Handle>:MMEMory:SEGMent:SAVE <"NewFileName ">[,<"SettingName">]
                                     [<"SegmentName ">]
```

Syntax 2:

```
:<Handle>:MMEMory:SEGMent:SAVE <"NewFileName">,
                                     <"AnalyzerSegmentName">
```

Parameters First parameter

<"NewFileName"> Specifies the file name under which the segments will be stored. The file format is according to the segment import and export syntax (see *"Segment Import and Export Language" on page 321*).

Optional second parameter (Syntax 1)

[<"SettingName">] If a setting name is specified, the segment is a local segment. With "" (empty string, just two quotes), the segment is assumed to be in the global segment pool.

Optional second parameter (Syntax 2)

[<"AnalyzerSegmentName">] Specifies a special segment Analyzer/Capture.p or Analyzer/ErrMem.p, where p is the port number of an output port.

Optional third parameter

[<"SegmentName">] Specifies a special segment. Absolute paths are allowed ("LocalSegments/segm", "GlobalSegments/segm", where segm corresponds to valid segments stored in the database under those nodes). The path names "Segments/segm" and "Analyzer/segm" are not valid.

Description The command is used to export segments to an external file.

Return Value None

Example :_test:MMEM:SEGM:SAVE "C:\TRAFFIC.TXT", "TEST1", "PAYLOAD"

In this example, the segment "PAYLOAD" located in the local setting "TEST1" is saved to the file "C:\TRAFFIC.TXT".

```
:_test:MMEM:SEGM:SAVE "C:\TRAFFIC2.TXT", "Analyzer/Capture.1"
```

In this example, the captured segment at port 1 ("Analyzer/Capture.1") is directly exported to the file "C:\TRAFFIC2.TXT".

:<Handle>:MMEMory:SEGMent:GET?

- Syntax** :<Handle>:MMEMory:SEGMent:GET? [<“SettingName”>][,<“SegmentName”>]
- Parameters** Optional first parameter
- [<“SettingName”>] If not specified, the global segment pool is addressed.
- Optional second parameter
- [<“SegmentName”>] If not specified, all segments in either the global or local segment pool (depending on [<“SettingName”>]) are addressed.
- Return Value** Returns an expression that contains the contents of the first-found segment(s) (vector definition, see “*Segment Import and Export Language*” on page 321). If the “SettingName” and the “SegmentName” are omitted, all segments are addressed in the global segment pool. If either “SettingName” or “SegmentName” is specified, a specific local segment is addressed.

Example :_test:MMEMory:SEGM:GET? "TEST1", "PAYLOAD"

might return:

Vector definition for "PAYLOAD" (see "*Segment Import and Export Language*" on page 321)

:<Handle>:MMEMory:SETTing:NAME?

- Syntax** :<Handle>:MMEMory:SETTing:NAME?
- Return Value** Returns the current setting name.
- Example** :_test:MMEM:SETT:NAME?
- might return the following current setting name:
- "TEST1"

:<Handle>:MMEMory:SETTing:LOAD

Syntax :<Handle>:MMEMory:SETTing:LOAD [<"SettingName">] [,<YDELay | NDELay | ODELay>]

Parameters Optional first parameter

[<"SettingName">] If not specified, the current setting is used. The setting at system power-up is "Default". If changes are stored with 'save-as', the current setting could be "TEST1".

YDELay Yes delay; load setting with cable delay parameters. This is the default.

NDELay No delay; load setting without cable delay parameters.

ODELay Only delay; load only cable delay parameters.

Description The command is used to load the current setting or a specified setting into the Agilent 81250 System's database.

Example :_test:MMEM:SETT:LOAD "TEST1"

:<Handle>:MMEMory:SETTing:SAVE

Syntax :<Handle>:MMEMory:SETTing:SAVE [<"SettingName">]

Parameters [**<"SettingName">**] If not specified, the changes are saved into the current setting. After system power-up, the name of the current setting is "Default".

Description The command is used to save into either the current setting or into a new setting.

Return Value None

Example :_test:MMEM:SETT:SAVE "TEST"

:<Handle>:MMEMory:SETTing:NEW

- Syntax** :<Handle>:MMEMory:SETTing:NEW
- Description** Resets and creates an ‘untitled’ environment. Starting from default values, a new setting can be created. To validate the new setting, it has to be ‘saved’ or ‘saved-as’ a into the Agilent 81250 System’s database.
- Return Value** None
- Example** :_test:MMEM:SETT:NEW

:<Handle>:MMEMory:SETTing:DELeTe

- Syntax** :<Handle>:MMEMory:SETTing:DELeTe <“SettingName”>
- Parameters** <“SettingName”> Setting to be deleted.
- Description** The command is used to delete the specified setting from the Agilent 81250 System’s database.
- Return Value** None
- Example** :_test:MMEM:SETT:DEL "TEST1"

:EDIT:SEGMENT(*) Subsystem

Syntax :<Handle>:EDIT:SEGMENT(*)

The :EDIT:SEGMENT(*) subsystem gives editing capabilities for creating new segments or updating existing segments. Data segments represent the pattern that must be generated for output and the expected data or captured data segments for input. The generator and analyzers are grouped to ports.

As a convention, each row in the data segment is called a **vector**. Each vector represents the data pattern that is generated or received at the one clock cycle. Each column in the data segment is called a **trace**. This represents the data stream of one output or input connector. Therefore, the width of a vector corresponds to the number of traces in the current hardware configuration.

One **state** is the information stored in one cell. Every vector has as many states as traces in width is the segment. The valid states depend on the coding for the segment. For two-bit codings, up to four states are valid. For one-bit codings, two different states exist.

The following diagram shows the vector and trace representation in a data segment from the Graphical User Interface:

	7	6	5	4	3	2	1	0
0x0	0	0	0	0	0	0	0	1
0x1	0	0	0	0	0	0	1	0
0x2	0	0	0	0	0	1	0	0
0x3	0	0	0	0	1	0	0	0
0x4	0	0	0	1	0	0	0	0
0x5	0	0	1	0	0	0	0	0
0x6	0	1	0	0	0	0	0	0
0x7	1	0	0	0	0	0	0	0

In order to work with one segment, you first have to open that segment. In return, you get an inspector number that is used for referencing that segment. This inspector number replaces the (*) symbol in the following calls. When no inspector number is given, the inspector number 1 is assumed by default.

Segments are stored in a segment pool, which is part of the system database. There is one segment pool with global scope and one segment pool with local scope.

- Segments in the local segment pools can only be accessed if the appropriate setting is loaded.
- Segments in the global segment pool can be accessed from any setting.

NOTE We recommend to set up the required data segments in the Segment Editor of the user interface and have these segments available in the system's database. In your program, you can open the segments.

Another possibility is to create the data segments using the Segment Import Language (see "*Segment Import and Export Language*" on page 321) and import the segments (see "[:<Handle>:MMEMORY:SEGMENT:LOAD" on page 92). This can ease your programming tasks and limits your time investment in coding.

[:<Handle>:EDIT:SEGMENT:OPEN?

Syntax [:<Handle>:EDIT:SEGMENT:OPEN? <"SegmentName">

Parameters <"SegmentName"> The name of a segment that is stored in the Agilent 81250 System's database.

Description Opens the specified segment.

For input and output ports: If the segment name is prefixed with 'GlobalSegments/', the global pool is searched; if the segment name is prefixed with 'LocalSegments/', the current setting is searched. If only a segment name is supplied, first the current setting is searched. If no segment of the specified name is found, the global segment pool is searched.

For output ports: If the segment name is prefixed with 'Analyzer/', the instrument memory is searched for all 'Capture.p' and 'ErrMem.p' segments of all analyzer ports (p is the port number). In Compare and Acquire around Error mode 'Capture.p' and 'ErrMem.p', segments are available for each port. In Capture Data mode, only 'Capture.p' segments are available. In Error Rate Measurement, there are no segments.

Return Value If the segment was successfully opened, the query returns the index of the segment inspector allocated to the segment. If the query returns zero, the segment could not be opened.

NOTE At low system clock rates (low frequencies), it takes some time till the system is ready to give access to the data segments. So, it is recommended to check the system state by the command :SGEN:GLOB:SYST:STATe? and wait until FINished is returned (see “: <Handle>:SGENeral:GLOBal:SYSTem:STATe?” on page 155). Then stop the system by the command :SGEN:GLOB:INIT:CONT OFF (see “: <Handle>:SGENeral:GLOBal:INITiate:CONTinuous” on page 154). Now it is possible to open the data segments.

Example :_test:EDIT:SEGM:OPEN? "PAYLOAD"

might return the following segment inspector index number:

3

As an example, the following command would save this segment under a new name:

:_test:EDIT:SEGM3:SAVE "PAYLOAD2"

:<Handle>:EDIT:SEGMENT(*):SAVE

Syntax :<Handle>:EDIT:SEGMENT(*):SAVE [<“SegmentName”>]

Parameters [<“SegmentName”>] Optional quoted string of the segment name with the target location for the new segment. The new segment can either be located in the “GlobalSegments/” pool or the “LocalSegments/” pool.

(*) Inspector number of the segment.

Description This command is used to save segments. When the “SegmentName” is given, it is a “save as”; if the “SegmentName” is omitted, then it is a “save” to the current segment name.

Example The following example saves the segment “test” that got the number “3” from the segment inspector (the number is the return value of the command :<hdl>:edit:segm:open?) as the new segment “payload” to the “GlobalSegments/” pool:

:_test:edit:segm3:save "GlobalSegments/payload"

:<Handle>:EDIT:SEGMENT(*):DELEte

- Syntax** :<Handle>:EDIT:SEGMENT(*):DELEte <"SegmentName">
- Parameters** <"SegmentName"> The name of a segment stored in the Agilent 81250 System's database.
- (*) The suffix (*) of SEGMENT is ignored.
- Description** Deletes the specified segment. If the segment name is prefixed with 'GlobalSegments/' the global pool is searched; if the segment name is prefixed with 'LocalSegments/', then the current setting is searched. If only a segment name is supplied, the current setting is searched. If no segment of the specified name is found, the global segment pool is searched.
- Example**

```
:_test:EDIT:SEGM:DEL "PAYLOAD" #Removes the segment "PAYLOAD"
                                #from the system's database
```

:<Handle>:EDIT:SEGMENT(*):CREate?

- Syntax** :<Handle>:EDIT:SEGMENT(*):CREate? <"SegmentName">, <SegmType>
- Parameters** <"SegmentName"> The name of a new segment to be created.
- <SegmType> Type of the segment to be created: MEMory | PRBS | PRWS | SFI5
- (*) The suffix (*) of SEGMENT is ignored.
- Description** Creates a new segment. The inspector number returned can then be used to refer to this segment. After being created, the segment is open and can be manipulated by means of the inspector number returned.
- If the segment already exists, this segment is opened.
- Only database segments can be created, not analyzer segments.
- The path for the segment to be created must be absolute. The pool names "LocalSegments/" and "GlobalSegments/" can be used.
- Segments that have been created during the current session but not yet saved in the database will not be listed when the MMEM subsystem is queried for them. However, the user can still work with them as normal segments.

Return Value Returns the inspector number of the segment just created.

Example :_test:EDIT:SEGM:CRE? "LocalSegments/letstry", MEM
might return the following segment inspector index number:
3

:<Handle>:EDIT:SEGMent(*):EXISts?

Syntax :<Handle>:EDIT:SEGMent(*):EXISts? <"SegmentName">

Parameters <"SegmentName"> The name of a segment.

(*) Inspector number of the segment.

Description Queries the existence of a segment. The segment might be an analyzer or a database segment.

Relative paths are only allowed for database segment. For other segments, the path must be absolute.

When a relative path is given, the LocalSegments pool is examined first. If the segment is not found there, the GlobalSegments pool is examined. If it is not found there, FALSE is returned

Return Value TRUE or FALSE

Example :_test:EDIT:SEGM:EXIS? "walking8"
might return:
TRUE

:<Handle>:EDIT:SEGMent(*):RPAth?

- Syntax** :<Handle>:EDIT:SEGMent(*):RPAth? <"SegmentName">
- Parameters** <"SegmentName"> The name of the segment (absolute or relative). This is an optional argument.
- (*) Inspector number of the segment. This is an optional suffix.
- Description** Returns the absolute path for one segment.
- To query for an open segment, you use the suffix for indicating its inspector number, but provide no arguments.
- To query about a not open segment, use the argument for indicating the name of the segment. In this case, all suffixes provided will be ignored.
- The name of the segment might be either an absolute or a relative path name. Of course, if an absolute path name is provided, the returned value will correspond to this argument.
- When a relative path is given, the LocalSegments pool will be examined first. If the segment is not found there, the GlobalSegments pool will be examined before returning an error.
- If neither argument nor suffix is provided, the inspector number 1 will be used by default.
- Return Value** <"AbsolutePathName"> The absolute path name of the input segment.

Example :_test:EDIT:SEGM:RPAT? "walking8"

might return:

"GlobalSegments/walking8"

:_test:EDIT:SEGM3:RPAT?

might return:

"LocalSegments/mysegment"

:<Handle>:EDIT:SEGMENT(*):CLOSE

Syntax :<Handle>:EDIT:SEGMENT(*):CLOSE

Parameters (*) Inspector number of the segment.

Description Closes the segment editor specified by the segment inspector index number without saving any changes made to the current segment name.

Example :_test:edit:segm3:close

:<Handle>:EDIT:SEGMENT(*):PATTERN:DATA

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:DATA
<trace1>,<vector1>,<trace2>,<vector2>,<stream>

Parameters <trace1> Number of start trace.

<vector1> Number of start vector.

<trace2> Number of end trace.

<vector2> Number of end vector.

<stream> Data stream to be set in the segment (hexadecimal string).

(*) Inspector number of the segment.

Description Sets data in a bounded rectangle in the segment.

New data can only be set for database segments. Attempting to set new data in an analyzer segment will cause an error.

The input data stream (<stream>) is a string of hexadecimal characters. The length of this string must be at least as many hexadecimal characters as needed to provide all the information required for the bounded rectangle. The format of this string is the same as explained for “:<Handle>:EDIT:SEGMENT(*):PATTERN:DATA?” on page 104.

If more characters are provided than required, they will be ignored. Also the trailing bits for the last character in every trace will be ignored.

Example :_test:EDIT:SEGM3:PATT:DATA 0,0,3,2,"FFFF"

:<Handle>:EDIT:SEGMENT(*):PATTERN:DATA?

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:DATA? <trace1>,<vector1>,<trace2>,<vector2>,<HEX|BIN>

Parameters <trace1> Number of start trace.

<vector1> Number of start vector.

<trace2> Number of end trace.

<vector2> Number of end vector.

<HEX|BIN> Specifies the format of the data stream returned. This can be a bit stream (BIN) or its conversion into a hexadecimal string—as a sequence of ASCII characters—(HEX).

(*) Inspector number of the segment.

Description Retrieves data from a bounded rectangle in a segment.

The data is returned in a stream. The first bytes in the stream correspond to all the data belonging to the first trace, followed by the data corresponding to the next trace, and so on.

Data for every trace is packed in an exact number of bytes. For example, if 5 vectors for every trace have been queried and the coding is 2 bits long, 10 bits will be needed for every trace data. For these 10 bits, 2 bytes are needed, and the “empty” 6 bits will be returned as 0s. After that, the 2 bytes for the next trace will appear in the data stream.

Every byte is filled starting from the most significant bits, so when there are spare bits in one byte, the less-significant bits will not be used. For more information on the coding, please refer to “:<Handle>:EDIT:SEGMENT(*):PATTERN:CODING?” on page 107.

If the HEX format is selected, these bytes will be directly transformed into hexadecimal ASCII characters. Every byte needs two hexadecimal characters.

If the BIN format is selected, some additional information is required.

BIN Format For BIN format, the returning stream will use the following format:

#abbbbcccccccccc where:

- a is the number of b's
- bbbb is the number of c's
- ccccc is the raw data; in the GUI, this raw data is presented as ASCII characters.

Return Value Returns the data stream corresponding to the region specified in the input.

Example :_test:EDIT:SEGM3:PATT:DATA? 0,0,3,2,HEX

might return the following segment data:


A040A0E0

:_test:EDIT:SEGM3:PATT:DATA? 0,0,3,2,BIN

might return the following segment data:

#9000000004 @ à

The following figure shows how the hex characters correspond to the segment data as shown in the user interface.

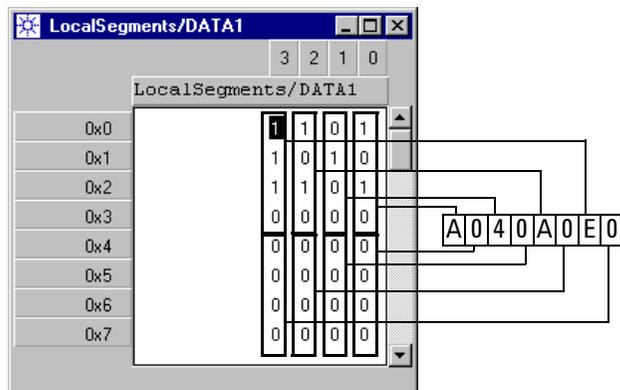

:<Handle>:EDIT:SEGMENT(*):PATTERN:CODING

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:CODING <"NewCoding">

Parameters <"NewCoding"> A quoted string of the new segment coding.

(*) Inspector number of the segment.

Description Sets the symbol coding to be used in this segment. It is typically used for setting the coding of a newly created segment.

If you want to convert the coding of an existing segment, use the :EDIT:SEGMENT(*):MOD:CONV command instead. See "<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:CONVERSE" on page 118 for more information.

New codings can only be set for database segments. Attempting to set a new coding in an analyzer segment will cause an error.

The only valid codings are "01" and "0 x1" (also "0 X1" is accepted).

- "01" results in a 1-bit coding for two states (low and high).
- "0 x1" results in a 2-bit coding for three states.

The order of the characters "0 x1" is particularly important as it implies the underlying binary values. Starting with 0, the coding assumes increasing order from left to right. The following table shows the mapping of state characters to binary segment data:

State Character	Binary Segment Data
0	00
'blank'	n/a
x	10
1	11

For example, the sequence 001xx will be coded as 00 00 11 10 10.

Example :_test:EDIT:SEGM3:PATT:CODING "01"

:<Handle>:EDIT:SEGMent(*):PATTern:CODing?

Syntax :<Handle>:EDIT:SEGMent(*):PATTern:CODing?

Return Value Returns the symbol coding used in this segment.

Example :_test:EDIT:SEGM3:PATT:COD?

might return the following segment coding:

"01"

:<Handle>:EDIT:SEGMent(*):PATTern:ERRor:FIRSt?

Syntax :<Handle>:EDIT:SEGMent*:PATTern:ERRor:FIRSt? <VECT | TRAC>, [NORMal | RVS]

Parameters [NORMal | RVS] Defines the direction of the search. Default is NORMal.

- NORMal

The search is started at trace 0, vector 0, and progresses in the incrementing trace, incrementing vector direction.

- RVS

The search is started at trace n-1, vector 0, and progresses in the decrementing trace, incrementing vector direction.

Return Value **t, v** Returns the coordinates (trace, vector) of the first found error. Returns coordinates -1, -1 if no error was found.

Example _TEST:SEGM1:PATT:ERR:FIRS? VECT,NORM

might return:

2,7

:<Handle>:EDIT:SEGMENT(*):PATTERN:ERROR:NEXT?

Syntax :<Handle>:EDIT:SEGMENT*:PATTERN:ERROR:NEXT? <trace>, <vector>, <VECT | TRAC>, [NORMAL | RVS]

Parameters As in the ERROR:FIRST? function, with the following additions:

<trace> Trace where the search starts.

<vector> Vector where the search starts.

Return Value See “:<Handle>:EDIT:SEGMENT(*):PATTERN:ERROR:FIRST?” on page 107.

Example `_TEST:SEGMENT1:PATTERN:ERROR:NEXT? 2,4,VECT,NORM`
might return:
`2,7`

:<Handle>:EDIT:SEGMENT(*):PATTERN:ERROR:PREVIOUS?

Syntax :<Handle>:EDIT:SEGMENT*:PATTERN:ERROR:PREVIOUS? <trace>, <vector>, <VECT | TRAC>, [NORMAL | RVS]

Parameters As in the ERROR:FIRST? function, with the following additions:

<trace> Trace where the search starts.

<vector> Vector where the search starts.

Return Value See “:<Handle>:EDIT:SEGMENT(*):PATTERN:ERROR:FIRST?” on page 107.

Example `_TEST:SEGMENT1:PATTERN:ERROR:PREV? 2,63,VECT,NORM`
might return:
`4,23`


:<Handle>:EDIT:SEGMENT(*):PATTERN:FIND:FIRST?

Syntax :<Handle>:EDIT:SEGMENT*:PATTERN:FIND:FIRST? <data>, <VECT | TRAC>, [NORMal | RVS]

Parameters <data> Data sequence to be searched for. It can be one of the following:

- Binary sequence (default, with optional “B” or “b” after the sequence)
- Octal sequence (with mandatory “O” or “o” after the sequence)
- Hexadecimal sequence (with mandatory “H” or “h” after the sequence)

<VECT | TRAC> Defines if the data sequence is searched for in traces or vectors.

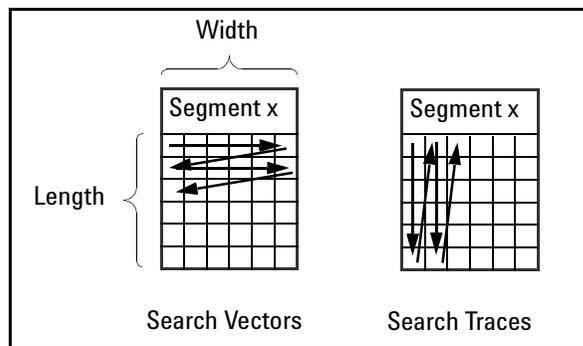


[NORMal | RVS] Defines if the direction of the search. Default is NORMal.

- NORMal
The search is started at trace 0, vector 0, and progresses in the incrementing trace, incrementing vector direction.
- RVS
The search is started at trace n-1, vector 0, and progresses in the decrementing trace, incrementing vector direction.

Return Value **d, v** Returns the digit index and vector index (comma-separated) of the starting point of the first found instance of the data sequence. Returns coordinates -1, -1 if the data sequence was not found.

The following graphic shows how the digit index and trace position are related.

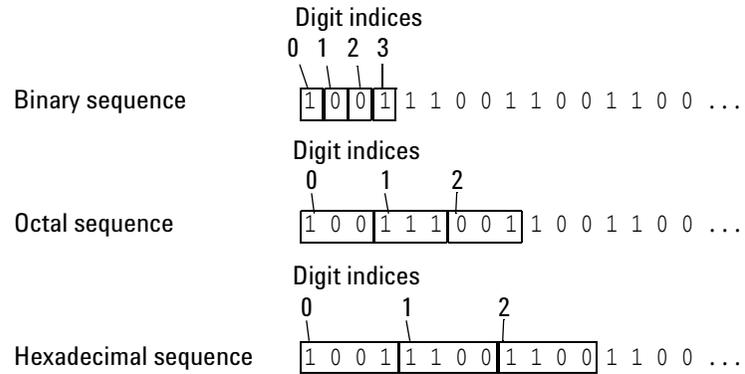

The following can be used to calculate the trace position from the returned digit index (d):

- Binary sequence
trace position = d
- Octal sequence
trace position = 3 * d
- Hexadecimal sequence
trace position = 4 * d

Example :_test:EDIT:SEG1:PATT:FIND:FIRS? "0101b", TRAC
 :_test:EDIT:SEG1:PATT:FIND:FIRS? "013h", TRAC
 :_test:EDIT:SEG1:PATT:FIND:FIRS? "037o", TRAC
 might return:
 1, 0

:<Handle>:EDIT:SEGMent(*):PATTern:FIND:NEXT?

Syntax :<Handle>:EDIT:SEGMent*:PATTern:FIND:Next? <digit>, <vector>, <data>, <VECT | TRAC>, [NORMal | RVS]

Parameters As in the FIND:FIRSt? function, with the following additions:

<digit> Defines the starting trace point of the search.

- Binary sequence
<digit> = trace point
- Octal sequence
<digit>= trace point / 3
- Hexadecimal sequence
<digit>= trace point / 4

<vector> Defines the vector where the search starts.

Return Value See “:<Handle>:EDIT:SEGMent(*):PATTern:FIND:FIRSt?” on page 109.

:<Handle>:EDIT:SEGMent(*):PATTern:FIND:PREVious?

Syntax :<Handle>:EDIT:SEGMent*:PATTern:FIND:Prev? <digit>, <vector>, <data>, <VECT | TRAC>, [NORMal | RVS]

Parameters As in the FIND:FIRSt? function, with the following additions:

<digit> Defines the starting trace point of the search.

- Binary sequence
<digit> = trace point
- Octal sequence
<digit>= trace point / 3
- Hexadecimal sequence
<digit>= trace point / 4

<vector> Defines the vector where the search starts.

Return Value See “:<Handle>:EDIT:SEGMent(*):PATTern:FIND:FIRSt?” on page 109.

:<Handle>:EDIT:SEGMENT(*):PATTERN:LENGTH?

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:LENGTH?

Parameters (*) Inspector number of the segment

Return Value Returns the number of vectors of the segment.

Example :_test:EDIT:SEGM3:PATT:LENG?

might return the following number of vectors of the specified segment:

80

:<Handle>:EDIT:SEGMENT(*):PATTERN:WIDTH?

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:WIDTH?

Parameters (*) Inspector number of the segment

Return Value Returns the numbers of traces of a segment.

Example :_test:EDIT:SEGM3:PATT:WIDT?

might return the following number of traces of the specified segment:

8

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:COPY

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:COPY StartTrace, StartVector, EndTrace, EndVector

Parameters **StartTrace** Number of start trace.

StartVector Number of start vector.

EndTrace Number of end trace.

EndVector Number of end vector.

(*) Inspector number of the segment.

Description Copies the bounded rectangle of data from the segment into the clipboard.

Example :_test:edit:segm3:patt:mod:copy 0,2,10,15

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:PASTE

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:PASTE StartTrace, StartVector

Parameters **StartTrace** Number of start trace.

StartVector Number of start vector.

(*) Inspector number of the segment.

Description Pastes the data currently stored in the clipboard to the specified segment.

If the number of vectors or traces from the initial state (defined by the starting trace and vector) up to the segment borders is smaller than the size of the data stored in the clipboard, the exceeding data from the clipboard will be ignored.

Attempting to paste data in an analyzer segment will cause an error.

Example :_test:EDIT:SEGM3:PATT:MOD:PASTE 0,76

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:FILL

- Syntax** :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:FILL StartTrace, StartVector, EndTrace, EndVector, State
- Parameters**
- StartTrace** Number of start trace.
 - StartVector** Number of start vector.
 - EndTrace** Number of end trace.
 - EndVector** Number of end vector.
 - State** New value to be set in this bounded region.
- (*) Inspector number of the segment.
- Description** Sets the bounded area of the segment with the same state value.
- State is an unsigned integer used to index the segment's coding for getting the new state to be used.
- For example, in coding "0 x1", the value of State might be an integer from 0 to 3. If a bigger integer is provided, the highest bits will be ignored and the least significant bits will be used to index the coding (for example, if "6" is provided, "2" will be used).
- Attempting to fill a region in an analyzer segment will cause an error.
- Example** :_test:EDIT:SEGM3:PATT:MOD:FILL 0,0,5,10,3

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:INVERT

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:INVERT StartTrace, StartVector, EndTrace, EndVector

Parameters **StartTrace** Number of start trace.

StartVector Number of start vector.

EndTrace Number of end trace.

EndVector Number of end vector.

(*) Inspector number of the segment.

Description Inverts the state information in the bounded area.

This command is only allowed in single-bit codings. Attempting to execute this command in multi-bit codings causes an error.

Attempting to invert data in a region in an analyzer segment causes an error.

For example, for the coding "01", after this command execution, all 0's will be changed into 1's and all the 1's will be changed into 0's in the area.

Example :_test:EDIT:SEGM3:PATT:MOD:INV 0,0,5,10

:<Handle>:EDIT:SEGMENT(*):PATTERN: MODIFY:MIRROR

- Syntax** :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:MIRROR StartTrace, StartVector, EndTrace, EndVector, <VECTOR|TRACE>
- Parameters**
- StartTrace** Number of start trace.
 - StartVector** Number of start vector.
 - EndTrace** Number of end trace.
 - EndVector** Number of end vector.
 - <VECTOR|TRACE>** Axis on which the mirror command will be performed.
 - (*)** Inspector number of the segment.
- Description** Flips the specified block about horizontal (VECTOR) or vertical axis (TRACE).
- Attempting to flip data in one region in an analyzer segment will cause an error.
- Example** :_test:EDIT:SEGM3:PATT:MOD:MIRR 0,0,5,10,VECT

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:INSERT

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:INSERT <Start>, <VECTOR|TRACE>, <BEFORE|AFTER>, HowMany

Parameters <Start> Number of start trace or vector.

<VECTOR|TRACE> What to insert, either traces or vectors.

<BEFORE|AFTER> Insert before or after the start trace or vector.

HowMany Number of vectors or traces to be inserted.

(*) Inspector number of the segment.

Description Inserts new traces or vectors into a segment. The segment is resized according with the number of new traces or vectors added.

The new vectors or traces will be initialized to 0.

Attempting to insert new data in an analyzer segment will cause an error.

Example _TEST:EDIT:SEG3:PATT:MOD:INS 2,VECT,AFT,3

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:DELETE

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:DELETE <Start>, <VECTOR | TRACE>, <HowMany>

Parameters <Start> Number of start trace or vector.

<VECTOR | TRACE> What to delete, traces or vectors.

<HowMany> Number of vectors or traces to be deleted.

(*) Inspector number of the segment.

Description Deletes traces or vectors from a segment. The segment is resized according to the number of new traces or vectors deleted.

Attempting to delete data from an analyzer segment causes an error.

Example :_test:EDIT:SEG3:PATT:MOD:DEL 2,VECT,3

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:CONVERSE

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:CONVERSE NewCoding, Mapping

Parameters **NewCoding** New coding for the segment.

Mapping Mapping between the old coding and the new coding.

(*) Inspector number of the segment.

Description This command changes the current coding for the segment and converts existing data in the segment according to the specified mapping.

The coding can be either "01" (binary) or "0x1" (binary with don't care).

The mapping depends on the coding, and corresponds with the desired new values.

Attempting to convert data from an analyzer segment will cause an error.

Examples The following examples illustrate how the command works:

To change a "01"-coded segment to "0x1"-coded, where "0" -> "0", "1" -> "x":

```
EDIT:SEGM1:PATT:MOD:CONV "0x1", "0x"
```

To invert a "01"-coded segment:

```
EDIT:SEGM1:PATT:MOD:CONV "01", "10"
```

To change a "0x1"-coded segment to "01"-coded, where "0" -> "0", "x" -> "1", "1" -> "1":

```
EDIT:SEGM1:PATT:MOD:CONV "01", "011"
```

To remap a "0x1"-coded segment, where "0" -> "x", "x" -> "0", "1" -> "1":

```
EDIT:SEGM1:PATT:MOD:CONV "0x1", "x01"
```

:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:SERIALIZE

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:SERIALIZE [NORMAL | RVS]

Parameters **NORMAL** Data is serialized in the order of the traces, from least significant bit to most significant bit (this is the default).

RVS Data is serialized in the reverse order (from most significant bit to least significant bit).

Description Serializes a parallel data stream. The optional direction parameter specifies the order in which the traces are to be considered. The following figure shows the differences between NORMAL and ReVerSe serializing.

Parallel	Serial (NORMAL)	Serial (RVS)
	a	d
	b	c
3 2 1 0	c	b
d b c a	d	a
h g f e	e	h
l k i j	f	g
	g	f
	h	e
	i	l
	j	k
	k	j
	l	i

Example :_test:EDIT:SEGMENT1:PATTERN:MODIFY:SERIALIZE RVS


:<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:DESERIALIZE

Syntax :<Handle>:EDIT:SEGMENT(*):PATTERN:MODIFY:DESERIALIZE <width> [,<phase>]

Parameters <width> Specifies the number of traces to be created for the parallel data stream.

[<phase>] (Optional) Specifies which trace is to be considered first (default is 0).

Description Deserializes a serial data stream. As shown below, <width> and <phase> determine how the serial data stream is deserialized to the parallel data stream.

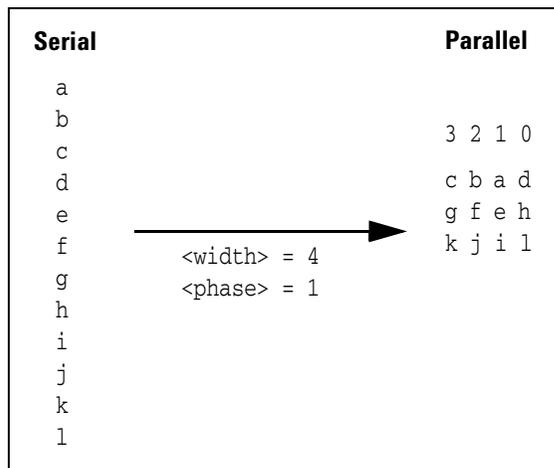

Example :_test:EDIT:SEGMENT1:PATTERN:MODIFY:DESERIALIZE 4, 1

:<Handle>:EDIT:SEGMENT(*):PARAMETER:LENGTH?

Syntax :<Handle>:EDIT:SEGMENT(*):PARAMETER:LENGTH?

Parameters (*) Inspector number of the segment.

Return Value Returns the length of the list of parameters available for this segment. The length of the list of parameters for analyzer segments is 0.

Example :_test:EDIT:SEGMENT3:PARAMETER:LENGTH?
= 1

:<Handle>:EDIT:SEGMent(*):PARAMeter:LIST?

Syntax :<Handle>:EDIT:SEGMent(*):PARAMeter:LIST?

Parameters (*) Inspector number of the segment.

Return Value Returns the list of parameters available for this segment. The list of parameters for analyzer segments is always empty.

For the list of parameters, see *“Predefined Parameter Names” on page 331*.

Example :_test:EDIT:SEGM3:PARA:LIST?

might return:

_Type

:<Handle>:EDIT:SEGMent(*):PARAMeter[:VALue]?

Syntax :<Handle>:EDIT:SEGMent(*):PARAMeter[:VALue]? <“ParamName”>

Parameters <“ParamName”> Name of the parameter.

For the list of parameters, see *“Predefined Parameter Names” on page 331*.

(*) Inspector number of the segment.

Return Value Returns the value for a specified parameter from the segment. Executing this command on analyzer segments causes an error.

Example :_test:EDIT:SEGM3:PARA? "_Type"

might return:

= (MEMORY)

:<Handle>:EDIT:SEGMENT(*):PARAMETER[:VALUE]

- Syntax** :<Handle>:EDIT:SEGMENT(*):PARAMETER[:VALUE] <"ParamName">, <(Expression)>
- Parameters** <"ParamName"> Name of the parameter. For the list of parameters, see *"Predefined Parameter Names" on page 331*.
- <(Expression)> New value for the parameter.
- (*) Inspector number of the segment.

Description Attempts to set the value for a specified parameter in the segment. Executing this command on analyzer segments causes an error.

Example :_test:EDIT:SEGM3:PARA "_Type", (PRBS)

:<Handle>:EDIT:SEGMENT(*):PARAMETER:REMOVE

- Syntax** :<Handle>:EDIT:SEGMENT(*):PARAMETER:REMOVE <"ParamName">
- Parameters** <"ParamName"> Name of the parameter. For the list of parameters, see *"Predefined Parameter Names" on page 331*.
- (*) Inspector number of the segment.

Description Removes a parameter from the list of parameters in the segment. Executing this command on analyzer segments causes an error.

Example :_test:EDIT:SEGM3:PARA:REM "_Type"

:<Handle>:EDIT:SEGMENT(*):TYPE

- Syntax** :<Handle>:EDIT:SEGMENT(*):TYPE <NewType>
- Parameters** <NewType> Available segment types: MEMORY|PRBS|PRWS|SFI5.
- (*) Inspector number of the segment.

Description Sets the segment type for the specified segment.

Example :_test:EDIT:SEGM3:TYPE MEM

:<Handle>:EDIT:SEGMENT(*):TYPE?

Syntax :<Handle>:EDIT:SEGMENT(*):TYPE?

Parameters (*) Inspector number of the segment.

Return Value Returns the segment type of the segment specified by the segment inspector index number (MEMORY|PRBS|PRWS|SFI5).

Example :_test:EDIT:SEG3:TYPE?

might return the following segment type:

MEM

[:CGROUP(*)] Subsystem

:<Handle>[:CGROUP(*)]

This subsystem allows to control system parameters on clock group level. The following subsystems are available:

- “[:CGROUP(*)]:MCLock Subsystem” on page 125
- “[:CGROUP(*)]:MODULE(*) Subsystem” on page 126
- “[:CGROUP(*)]:MODULE(*):CONNECTOR(*) Subsystem” on page 129
- “[:CGROUP(*)][:SOURCE]:TRIGGER Subsystem” on page 134

:<Handle>[:CGRoup(*)]:CINFormation?

Syntax :<Handle>[:CGRoup(*)]:CINFormation? <SHORt | DETailed>

Return Value This query returns the clock group configuration information. The response is an expression according to the following syntax:

```

<ClockGrpInfo> ::= "(" <ModuleInfo> ("," <ModuleInfo>)* ")"
<ModuleInfo>   ::= "(" <ProductNr> "," <SpeedClass> ["," <SerNr>
                    "," <IDNr>] "," <ConnInfo> ("," <ConnInfo>)* ")"
<ConnInfo>    ::= "(" <ProductNr> "," <SpeedClass> "," "Type" [","
                    <SerNr> "," <IDNr> "," <ConnNr>] ")"
<ProductNr>   ::= for example, "E4838A"
<SpeedClass>  ::= for example, 660
<Type>        ::= "ANALYZER" | "GENERATOR"
<SerNr>       ::= serial number (0 if not available)
<IDNr>        ::= identification number (0 if not available)
<ConnNr>      ::= "S1" | "D1" | "D2"
                S1: single frontend
                D1: first connector of a dual frontend
                D2: second connector of a dual frontend

```

The optional syntax elements only appear if DETailed is selected.

Example :_test:CINF? SHOR

might return, for example (formatted here only for readability):

```

((E4805B,660),
 (E4861A,2640,
  (E4863A,2640,ANALYZER),
  (E4862A,2640,GENERATOR)),
 (E4861A,2640,
  (E4863A,2640,ANALYZER),
  (E4862A,2640,GENERATOR)))

```

[:CGROUP(*)]:MCLock Subsystem

Syntax :<Handle>[:CGROUP(*)]:MCLock

This tree provides the commands which set or query the “master” system clock module in the Agilent 81250 System. It is possible to have more than one clock module installed, to have more than one “virtual” instrument. It is then possible to synchronize these “virtual” instruments, by defining one as the “master” clock generator.

:<Handle>[:CGROUP(*)]:MCLock:SOURce[:VALue]

Syntax :<Handle>[:CGROUP(*)]:MCLock:SOURce[:VALue] <ON | OFF>

Description Because it is possible to have more than one clock module in the Agilent 81250 System, this command controls which of the clock modules generates the “master” clock.

Example :_test:CGR1:MCL:SOUR ON

:<Handle>[:CGROUP(*)]:MCLock:SOURce[:VALue]?

Syntax :<Handle>[:CGROUP(*)]:MCLock:SOURce[:VALue]?

Return Value State of the clock module of the specified clock group. When ON is returned, this is the “master” clock module in the Agilent 81250 System.

Example :_test:cgroup1:mcl:sour?
might return:
ON

[:CGRoup(*)]:MODule(*) Subsystem

Syntax :<Handle>[:CGRoup(*)]:MODule(*)

This tree provides a set of commands which co-operate with a single module.

:<Handle>[:CGRoup(*)]:MODule(*): CINformation?

Syntax :<Handle>[:CGRoup(*)]:MODule(*)CINformation? <SHORT | DETailed>

Return Value This query returns the module configuration information, including the frontends. The response is an expression according to the following syntax:

```
<ModuleInfo> ::= "("<ProductNr> "," <SpeedClass> ["," <SerNr> ","
                <IDNr>] "," <ConnInfo> ("," <ConnInfo>)* ")"
<ConnInfo>   ::= "("<ProductNr> "," <SpeedClass> "," "Type" [","
                <SerNr> "," <IDNr> "," <ConnNr>] ")"
<ProductNr>  ::= for example, "E4838A"
<SpeedClass> ::= for example, 660
<Type>       ::= "ANALYZER" | "GENERATOR"
<SerNr>      ::= serial number (0 if not available)
<IDNr>       ::= identification number (0 if not available)
<ConnNr>     ::= "S1" | "D1" | "D2"
```

S1: single frontend

D1: first connector of a dual frontend

D2: second connector of a dual frontend

The optional syntax elements only appear if DETailed is selected.

Example :_test:MOD2:CINF? DET

might return for example (formatted here only for readability):

```
(E4861A,2640,"DE40701397","DE40701397/0",
 (E4863A,2640,ANALYZER,"DE40701316","DE40701316/0",S1),
 (E4862A,2640,GENERATOR,"DE40701738","DE40701738/0",S1))
```

:<Handle>[:CGRoup(*)]:MODule(*):TYPE?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):TYPE?

Returns the product number of the specified module in a quoted string.

Example :_test:CGRoup1:MOD1:TYPE?

might return:

"4805B"

:<Handle>[:CGRoup(*)]:MODule(*):SLOT?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):SLOT?

Returns the slot number in which the specified module is located.

Example :_test:CGR1:MOD1:SLOT?

might return:

3

**:<Handle>[:CGRoup(*)]:MODule(*):
FRAME?**

Syntax :<Handle>[:CGRoup(*)]:MODule(*):FRAME?

Returns the frame number to which the specified module belongs.

Example :_test:CGR1:MOD1:FRAME?

might return:

1

:<Handle>[:CGRoup(*)]:MODule(*):NAME?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):NAME?

Returns the name of the specified module.

Example :_test:CGR1:MOD1:NAME?

might return:

"E4805B_01"

:<Handle>[:CGROUP(*):MODULE(*): CNAMES?

Syntax :<Handle>[:CGROUP(*):MODULE(*):CNAMES?

Returns a quoted list of connector names.

The connector names are 7-digit quoted strings, defined according to connector, module and clock group. The following syntax is used:

ggmmccc

gg represents the clock group, mm represents the module, ccc represents the connector.

Example :_test:CGR1:MOD1:CNAM?

might return:

"0102001", "0102002", "0102003", "0102004"

[:CGROUP(*):MODULE(*): CONNECTOR(*) Subsystem

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*) subsystem

This tree provides administration and calibration commands available only at connector level.

Further commands are available at connector level (commands for timing, level, input and output parameters and for data formats). Because these commands are also available at port and terminal levels, they are described separately in sections for each parameter type.

:<Handle>[:CGROUP(*):MODULE(*): CONNECTOR(*)):CINFORMATION?

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*)):CINFORMATION?
<SHORT | DETAILED>

Return Value This query returns the connector configuration information. The response is an expression according to the following syntax:

```
<ConnectorInfo> ::= ("<ProductNr> ", "<SpeedClass> ", "<Type>"
                  [ "<SerNr> ", "<IDNr> ", "<ConnNr> ] ")
<ProductNr>    ::= for example, "E4838A"
<SpeedClass>   ::= for example, 660
<Type>         ::= "ANALYZER" | "GENERATOR"
<SerNr>        ::= serial number (0 if not available)
<IDNr>         ::= identification number (0 if not available)
<ConnNr>       ::= "S1" | "D1" | "D2"

                  S1: single frontend
                  D1: first connector of a dual frontend
                  D2: second connector of a dual frontend
```

The optional syntax elements only appear if DETAILED is selected.

Example :_test:MOD2:CONN1:CINF? DET

might return for example:

```
(E4863A,2640,ANALYZER,"DE40701316","DE40701316/0",S1)
```

:<Handle>[:CGRoup(*):MODule(*):CONNector(*):TYPE?

Syntax :<Handle>[:CGRoup(*):MODule(*):CONNector(*):TYPE?

Returns the product number of the frontend to which the connector belongs. This value is returned in a quoted string.

Example :_test:CGR1:MOD1:CONN1:TYPE?

might return:

"E4863A"

:<Handle>[:CGRoup(*):MODule(*):CONNector(*):NAME?

Syntax :<Handle>[:CGRoup(*):MODule(*):CONNector(*):NAME?

Returns the name of the specified connector as a 7-digit quoted string according to connector, module and clock group. The following syntax is used:

ggmmccc

gg represents the clock group, mm represents the module, ccc represents the connector.

Example :_test:CGR1:MOD1:CONN1:NAME?

might return:

"0102001"

The above query returns the name of connector 1 in module 2 of clock group 1.

:<Handle>[:CGRoup(*):MODule(*):CONNector(*):TNAME?

Syntax :<Handle>[:CGRoup(*):MODule(*):CONNector(*):TNAME?

Returns the terminal name to which this connector is connected. An empty "" string is returned if the connector is not connected.

Example :_test:CGR1:MOD1:CONN1:TNAME?

might return:

"Data1"

:<Handle>[:CGROUP(*):MODULE(*): CONNECTOR(*):CALIBRATION:CDELAY

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):CALIBRATION:CDELAY <Cable Delay>

Parameters <NRf> Cable Delay value.

Sets a cable delay for the specified connector to synchronize it with other signals applied to the DUT terminals.

NOTE Delay Auto Calibration must be performed before the cable delay can be set.

Example :_test:MOD1:CONN1:CAL:CDEL 6.5e-9

:<Handle>[:CGROUP(*):MODULE(*): CONNECTOR(*):CALIBRATION:CDELAY?

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):CALIBRATION:CDELAY?

Return Value Returns the current cable delay for the specified connector of the specified module.

Example :_test:MOD1:CONN1:CAL:CDEL?

might return:

6.500000E-009

:<Handle>[:CGROUP(*):MODULE(*): CONNECTOR(*):CALIBRATION:ZDELAY

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):CALIBRATION:ZDELAY <Zero Delay>

Sets a zero delay for the specified connector of the specified module.

Parameters <Zero Delay> Zero delay value.

NOTE Delay Auto Calibration must be executed before zero delay can be set.

Related Commands • “:<Handle>:SGENERal:GLOBal:CALibration:SELF DELay” on page 143

Example :_test:CGR1:MOD1:CONN:CAL:ZDEL 1.0e-9

:<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):CALibration:ZDELay?

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):CALibration:ZDELay?

Return Value Returns the current zero delay for the specified connector.

Example :_test:cgr1:mod1:conn1:cal:zdel?

might return:

1.000000E-009

:<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):SPECies[:VALue]?

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):SPECies?

Return Value Returns a comma-separated list of the species states that are supported by the connector. This can be either ELECtric or OPTic.

Example :_test:cgr1:mod1:conn1:spec?

might return:

ELEC,OPT

:<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):SPECies:STATe

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):SPECies:STATe
<ELEC|OPT>

Parameters <ELEC|OPT> Switches the connector into either electrical (ELEC) or optical (OPT) mode.

NOTE This command can only be executed when the connector is not connected to any port.

Example :_test:cgr1:mod1:conn1:spec:stat elec

:<Handle>[:CGROUP(*):MODULE(*): CONNECTOR(*):SPECIES:STATE?

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):SPECIES:STATE?

Return Value Returns the current species of the connector. Possible return values are electrical (ELEC) or optical (OPT).

Example :_test:cgr1:mod1:conn1:spec:stat?

might return:

ELEC

[:CGRoup(*)][:SOURce]:TRIGger Subsystem

:<Handle>[:CGRoup(*)][:SOURce]:TRIGger

This command subsystem is used to set the trigger or strobe output parameters.

[:<Handle>[:CGRoup(*)][:SOURce]:TRIGger: DELay

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:DELay <NRF>

The delay of the trigger output signal can be varied with this command. For frequencies ≤ 330 MHz in the range of 0 to 360 ns, for frequencies >330 MHz in the range of 0 to 3.3 ns

Example :_test:CGR1:TRIG:DEL 2e-9

[:<Handle>[:CGRoup(*)][:SOURce]:TRIGger: DELay?

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:DELay?

Return Value Returns the current delay of the trigger output signal.

Example :_test:CGR1:TRIG:DEL?

might return:

2.000000E-009

[:<Handle>][:CGRoup(*)][:SOURce]:TRIGger: MUX

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:MUX <NRf>

Parameters <NRf> MUX factor = frequency multiplier factor for the individual connector

In addition to the “system” MUX factor (Segment Resolution) it is possible to set the frequency multiply factor for the trigger output, as for individual connectors, to generate multiples or fractions of 2 of the frequency of the data streams, like $f/2$ or $2f$ etc. The default value is 1, or $1/4$ if the system is equipped with E4861A modules only. Valid values are:

0.0625 ($1/16$), 0.125 ($1/8$), 0.25 ($1/4$), 0.5 ($1/2$), 1, 2, 4, 8, 16

The range of this parameter depends on the value of the “system” MUX factor (Segment Resolution). See “[:<Handle>]:SGENERal:GLOBal:MUX” on page 146.

Example :_test:CGR1:TRIG:MUX 2

[:<Handle>][:CGRoup(*)][:SOURce]:TRIGger: MUX?

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:MUX?

Return Value The MUX factor associated with the trigger output.

Example :_test:CGR1:TRIG:MUX?

might return:

2

[:<Handle>][:CGRoup(*)][:SOURce]:TRIGger: OUTPut[:STATe]

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:OUTPut[:STATe] ON

Parameters ON Resets the protection circuit of the trigger output of an E4809A clock module. The hardware switches the trigger output in case of an overload. This command switches it back on.

Example :_test:CGR1:TRIG:OUTP ON

:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:OUTPut[:STATe]?

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:OUTPut[:STATe]?
<NFORce|FORCe>

Return Value Returns the state of the E4809A clock module trigger output. The optional parameter **FORCe|NFORce** determines how the query is executed (see following text).

Parameters <NFORce|FORCe> Defines how the query is executed:

- NFORce
Default value. Only the firmware is queried for the current state.
- FORCe
When FORCe is entered, the firmware checks the current condition in the hardware. This is required to make sure that the trigger output is really switched on, or to check if the protection circuit within the trigger output has turned off the channel to protect it from damage.

Example :_test:CGR1:TRIG:OUTP? FORC
might return:
OFF

:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:HIGH

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:HIGH <NRf>

Parameters <NRf> The upper voltage level of the trigger output signal.

Example :_test:CGR1:TRIG:VOLT 2

:<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:HIGH?

Syntax :<Handle>[:CGRoup(*)][:SOURce]:TRIGger:VOLTage[:LEVel][:IMMediate]:HIGH?

Returns the upper voltage level of the trigger output signal.

Example :_test:CGR1:TRIG:VOLT?

might return:

2.000000E+000

[:<Handle>][:CGROUP(*)][:SOURCE]:TRIGGER: VOLTage[:LEVEL][:IMMEDIATE]:LOW

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:VOLTage[:LEVEL][:IMMEDIATE]:LOW
<NRf>

Parameter <NRf> The lower voltage level of the trigger output signal.

Example :_test:CGR1:TRIG:VOLT:LOW -1

[:<Handle>][:CGROUP(*)][:SOURCE]:TRIGGER: VOLTage[:LEVEL][:IMMEDIATE]:LOW?

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:VOLTage[:LEVEL][:IMMEDIATE]:
LOW?

Returns the lower voltage level of the trigger output signal.

Example :_test:CGR1:TRIG:VOLT:LOW?

might return:

-1.000000E+000

[:<Handle>][:CGROUP(*)][:SOURCE]:TRIGGER: TVOLTage

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:TVOLTage <NRf>

Specifies the termination voltage of a trigger output connector. The
-2.1 V to +3.1 V.

Example :_test:CGROUP1:SOURCE:TRIGGER:TVOLTAGE -2

[:<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:TVOLTage?

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:TVOLTage?

Return Value Returns the current termination voltage of the trigger output connector.

Example :_test:CGROUP1:SOURCE:TRIGGER:TVOLTAGE?
might return:
-2.000000E+000

[:<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:IMPedance:EXTernal

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:IMPedance:EXTernal <NRf>

Description The external termination impedance can be specified by this command. Any negative value is interpreted as into “open”.

Example :_test:CGR1:TRIG:IMP 500

[:<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:IMPedance:EXTernal?

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:IMPedance:EXTernal?

Return Value Returns the current programmed external termination impedance (load impedance).

Example :_test:CGR1:TRIG:IMP?
might return:
5.000000E+002

[:<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:MODE

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:MODE SEQUencer | CGENeration

Description This command is used to select the source of the trigger output. It is possible to derive the source of the trigger signal from the sequencer circuit (SEQUencer) or from the clock generation circuit (CGENeration).

Example :_test:CGROUP1:TRIGGER:MODE SEQ

[:<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:MODE?

Syntax :<Handle>[:CGROUP(*)][:SOURCE]:TRIGGER:MODE?

Return Value Returns the actual source used for the trigger signal.

Example :_test:CGR1:TRIG:MODE?

might return:

SEQ

:SGENeral Subsystem

Syntax :<Handle>:SGENeral

The :SGENeral subsystem represents the General Scheme. It represents a DUT with several ports. A port represents a collection of input or output connections (terminals). With these commands, you model your specific setup by defining data or pulse ports, naming the terminals and connecting the terminals of the DUT with the output and input resources of the Agilent 81250 System. The used virtual instrument of the Agilent 81250 System is represented by the “[:CGRoup(*)] Subsystem” on page 123.

The following subsystems are available:

- “:SGENeral:INFormation Subsystem” on page 141
- “:SGENeral:GLOBal Subsystem” on page 142
- The :SGENeral:PDATA(*) and :SGENeral:PPULSE(*) subsystems allow to specify timing, level, input and output parameters and data formats on port and terminal levels. Furthermore, port and terminal administration commands are available for pulse and data ports.

The :SGENeral:PDATA(*) subsystem also provides commands for error analysis.

These commands are described separately in sections for each parameter type or command group.

- The :<Handle>:SGENeral:CONNECT subsystem provides commands for connector administration for pulse and data ports. They are available at port and terminal level and are described in “Connector Administration Commands” on page 309.

:SGENeral:INFormation Subsystem

Syntax :<Handle>:SGENeral:INFormation

This subsystem provides information about the general scheme.

:<Handle>:SGENeral:INFormation: PCLasses?

Syntax :<Handle>:SGENeral:INFormation:PCLasses?

Return Value Returns the list of implemented port classes in a comma-separated quoted string list.

Example :_test:SGENeral:INFormation:PCLasses?

returns:

"DATA", "PULSE"

:SGENeral:GLOBal Subsystem

Syntax :<Handle>:SGENeral:GLOBal

This subsystem provides commands to modify system parameters. These commands affect the entire system including any frames connected via MXI.

In addition to the top-level commands, this subsystem contains further subsystems:

- “:SGENeral:GLOBal:CONFIgure Subsystem” on page 151
- “:SGENeral:GLOBal:INITiate:CONTInuous Subsystem” on page 154
- “:SGENeral:GLOBal:SYSTem Subsystem” on page 155
- “:SGENeral:GLOBal:SEQuence Subsystem” on page 156
- “:SGENeral:GLOBal:TRIGger Subsystem” on page 173
- “:SGENeral:GLOBal:ARM Subsystem” on page 179

:<Handle>:SGENeral:GLOBal:CONNect

Syntax :<Handle>:SGENeral:GLOBal:CONNect <ON | OFF>

Description Connects or disconnects all enabled connectors of the Agilent 81250 System at the same time.

Example :_test:SGEN:GLOB:CONN OFF

:<Handle>:SGENeral:GLOBal:CONNect?

Syntax :<Handle>:SGENeral:GLOBal:CONNect?

Return Value Returns the actual connection status of the enabled connectors.

Example :_test:SGEN:GLOB:CONN?

might return:

OFF

:<Handle>:SGENeral:GLOBal:CALibration:PUSe PASSive

Syntax :<Handle>:SGENeral:GLOBal:CALibration:PUSe PASSive

Description Instead of assuming an active probe, this option uses the customer-provided levels. This is useful when you use long cables, for example for testing the pins of an integrated circuit.

Example :_test:SGEN:GLOB:CAL:PUS PASS

:<Handle>:SGENeral:GLOBal:CALibration:SELF DELay

Syntax :<Handle>:SGENeral:GLOBal:CALibration:SELF DELay

Description Any time frontends were exchanged in a module, the system must be autocalibrated after a 30-minute warmup period. Delay Auto Calibration must be performed before Zero Adjustment or Cable Adjustment.

Related Commands

- “:CALibration:CDELay” on page 303
- “:<Handle>[:CGRoup(*):MODule(*):CONNector(*):CALibration:ZDELay” on page 131

Example :_test:SGEN:GLOB:CAL:SELF DEL

:<Handle>:SGENeral:GLOBal:DOFFset

Syntax :<Handle>:SGENeral:GLOBal:DOFFset <DelayOffset>

Parameters <DelayOffset> A numeric value out of the specified range, for example, 10e-9.

This command specifies an offset value to the fixed delay for all connectors. So, it is possible to set negative delays for individual connectors to achieve setup and hold times behavior.

Example :_test:SGEN:GLOB:DOFF 10e-9

:<Handle>:SGENeral:GLOBal:DOFFset?

- Syntax** :<Handle>:SGENeral:GLOBal:DOFFset?
- Return Value** The current set delay offset.
- Example** :_test:SGEN:GLOB:DOFF?
might return:
1.000000E-008

:<Handle>:SGENeral:GLOBal:FETCh:ERRor:ANY?

- Syntax** :<Handle>:SGENeral:GLOBal:FETCh:ERRor:ANY?
- Description** The query returns 0 for no errors, or 1 if an error was found in the system. This can be used to increase program speed. Uploading of memory segments can be completely avoided, when it is known that there are no errors at all.
- Example** :_test:SGEN:GLOB:FETC:ERR:ANY?
might return:
0

:<Handle>:SGENeral:GLOBal:PERiod

- Syntax** :<Handle>:SGENeral:GLOBal:PERiod <Period>
- Parameters** <Period> A numeric value out of the specified range, e.g. 10e-9.
Sets the period of the Agilent 81250 System.
- NOTE** The period at an individual connector depends on the frequency multiply factor chosen for this connector.
- Example** :_test:SGEN:GLOB:PER 10e-9

:<Handle>:SGENeral:GLOBal:PERiod?

Syntax :<Handle>:SGENeral:GLOBal:PERiod?

Return Value The currently set clock period.

Example :_test:SGEN:GLOB:PER?

might return:

1.000000E-008

:<Handle>:SGENeral:GLOBal:FREQuency

Syntax :<Handle>:SGENeral:GLOBal:FREQuency <Frequency>

Parameters <Frequency> A numeric value out of the specified range, e.g. 100E6.

Sets the frequency of the Agilent 81250 System.

NOTE The frequency at an individual connector depends on the frequency multiply factor chosen for this connector.

Example :_test:SGEN:GLOB:FREQ 100E6

:<Handle>:SGENeral:GLOBal:FREQuency?

Syntax :<Handle>:SGENeral:GLOBal:FREQuency?

Return Value The currently set clock frequency.

Example :_test:SGEN:GLOB:FREQ?

might return:

1.000000E008

:<Handle>:SGENeral:GLOBal:MUX?

Syntax :<Handle>:SGENeral:GLOBal:MUX?

Return Value The current 'MUX' factor (Segment Resolution).

See ":<Handle>:SGENeral:GLOBal:MUX" on page 146 for details.

Example :_test:SGEN:GLOB:MUX?

might return:

4

:<Handle>:SGENeral:GLOBal:MUX

Syntax :<Handle>:SGENeral:GLOBal:MUX <MUX factor>

Parameters **<MUX factor>** MUX factor equals the Segment Resolution. With this command, the global settings are defined. The Segment Resolution defines the Frequency Multiplier Range, the min/max System Clock Rate and the Memory Depth of the data stream.

For E4832A modules, valid values for the MUX Segment Resolution are 1, 2, 4, 8, and 16.

For E4861A modules, valid values are 16, 32, and 64.

For E4861B modules, valid values are 1, 2, 4, 8, 16, 32, 64, and 128.

For E4866A and E4867A modules, the only valid value is 256.

For N4872A, N4873A, N4874A and N4875A modules, valid values are 32, 64, 128, 256, and 512.

Different values will be rounded off/on to the next valid value. Each connector can be set to an individual frequency multiply factor, see the timing parameter command ":MUX" on page 201.

The E4832A module has a memory capacity of 2 MB per channel.

System Clock Frequency Mbit/s	Segment Resolution bits	Memory Depth bits	Possible Frequency Multipliers
≤ 42.1875	1	131,008	1, 2, 4, 8, 16
≤ 84.375	2	262,016	1/2, 1, 2, 4, 8
≤ 168.750	4	524,032	1/4, 1/2, 1, 2, 4
≤ 337.500	8	1,048,064	1/8, 1/4, 1/2, 1, 2
≤ 675.000	16	2,097,152	1/16, 1/8, 1/4, 1/2, 1

NOTE For E4832A modules, the delay vernier and the functions for automatic analyzer sampling delay adjustment require that the minimum segment resolution of the desired system clock frequency is used.

The E4861A module has a memory capacity of 8 MB per channel.

System Clock Frequency Mbit/s	Segment Resolution bits	Memory Depth bits	Possible Frequency Multipliers
337.500 – 675.000	16	2,097,152	1, 2, 4
≤ 1,350.000	32	4,194,304	1/2, 1, 2
≤ 2,700.000	64	8,388,608	1/4, 1/2, 1

The E4861B module has a memory capacity of 16 MB per channel.

System Clock Frequency (Mbit/s)	Segment Resolution (bits)	Memory Depth (bits)	Possible Frequency Multipliers
20.834 to 41.666	1	131,072	1, 2, 4, 8, 16, 32, 64, 128
≤ 82.333	2	262,144	1/2, 1, 2, 4, 8, 16, 32, 64
≤ 166.666	4	524,288	1/4, 1/2, 1, 2, 4, 8, 16, 32
≤ 333.333	8	1,048,576	1/8, 1/4, 1/2, 1, 2, 4, 8, 16
≤ 666.666	16	2,097,152	1/16, 1/8, 1/4, 1/2, 1, 2, 4, 8
≤ 1,333.333	32	4,194,304	1/32, 1/16, 1/8, 1/4, 1/2, 1, 2, 4
≤ 2,700.000	64	8,388,608	1/64, 1/32, 1/16, 1/8, 1/4, 1/2, 1, 2
≤ 3,350.000	128	16,777,216	1/128, 1/64, 1/32, 1/16, 1/8, 1/4, 1/2, 1

The E4866A and E4867A modules have a memory capacity of 32 MB per channel.

System Clock Frequency (Gbit/s)	Segment Resolution (bits)	Memory Depth (bits)	Possible Frequency Multipliers
9.5 to 10.8	256	33,554,432	1

The N4872 to N4875 modules have a memory capacity of 64 MB per channel.

System Clock Frequency (Gbit/s)	Segment Resolution (bits)	Memory Depth (bits)	Possible Frequency Multipliers
≤ 1.350	32	4,194,304	1, 2, 4, 8, 16
≤ 2.700	64	8,388,608	1/2, 1, 2, 4, 8
≤ 5.400	128	16,777,216	1/4, 1/2, 1, 2, 4
≤ 10.800 (N4874/75A ≤ 7,000)	256	33,554,432	1/8, 1/4, 1/2, 1, 2
≤ 13.500 (N4874/75A ≤ 7,000)	512	67,108,864	1/16, 1/8, 1/4, 1/2, 1

The desired system clock frequency determines the minimum segment resolution. As long as the segment resolution is less than 16 (or 64 for E4861A modules), it is possible to choose a higher general segment resolution. This increases the usable memory and simultaneously decreases the sequencer clock frequency.

For more details, see “*Frequency Multiplier and Segment Resolution*” in the *System User Guide*.

The following table illustrates the relationships between the different values (shown for an E4832A module):

Segment Resolution	Frequency Multiplier Range (FMR) ^a	Memory Depth ^b	System Clock Rates
1 bit (=1)	1, 2, 4, 8, 16	128 Kbit	≤ 42.1875 MHz
2 bits (=2)	1/2, 1, 2, 4, 8	256 Kbit	≤ 84.375 MHz
4 bits (=4)	1/4, 1/2, 1, 2, 4	512 Kbit	≤ 168.75 MHz
8 bits (=8)	1/8, 1/4, 1/2, 1, 2	1 Mbit	≤ 337.5 MHz
16 bits (=16)	1/16, 1/8, 1/4, 1/2, 1	2 Mbit	≤ 675 MHz

^a This is the range of multiples and fractions that can be used at individual connectors. If you have most of your signals at 40 MHz and your pattern lengths are less than 128 Kbit, then you can choose segment resolution 1. You have the chance to set individual connectors to a multiple of this general setting. For example, selecting 16 as the multiply factor for a connector gives you 2 Mbit memory depth and 640 MHz with a segment resolution of 16.

^b Subtract 32 x segment resolution, as this memory space is occupied by a 2⁵-1 PRxS and the sequencing initialization.

Example :_test:SGEN:GLOB:MUX 4

:<Handle>:SGENeral:GLOBal:PLL:DState?

Syntax :<Handle>:SGENeral:GLOBal:PLL:DState?

Description Determines the PLL (Phase Locked Loop) state. The PLL circuit locks on external clock signals. PLL:DState indicates whether the internal and external signals are locked (that is, whether they have the same period and phase) and returns a list of unlocked modules.

Return Value **LOCKed** Indicates that the internal and external signals are locked.

UCDR (Unlocked Clock Data Recovery) Indicates that the clock data recovery (CDR) circuit could not synchronize on the incoming data stream. Because the generated clock signal is undefined, it is useless to continue the test. You may consider using an external clock.

UDATa (Unlocked DATa, only available for the E4869B and N4872A to N4875A modules) Indicates that the input clock is not stable enough.

Any return value other than **LOCKed** indicates that the internal and external signals are not locked. In this case, you can do the following to identify the problem:

- Check the physical connection to the module.
- Check the level parameter or the frequency of the supplied signal.

The supplied signal should be roughly equal to the internal frequency of the module. You can check this in the GUI.

Example :_test:SGEN:GLOB:PLL:DST?

might return:

LOCK, (@) (the internal and external signals are locked)

LJNL, (@0101001) (the first central module C1M1C1 is unlocked)

:<Handle>:SGENeral:GLOBal:PLL:STATe?

Syntax :<Handle>:SGENeral:GLOBal:PLL:STATe?

Description Determines the PLL (Phase Locked Loop) state. The PLL circuit locks on external clock signals. PLL:STATe indicates whether the internal and external signals are locked (that is, that they have the same period and phase).

Return Value **LOCKed** Indicates that the internal and external signals are locked.

UCDR (Unlocked Clock Data Recovery) If this value is returned, then the clock data recovery (CDR) circuit could not synchronize on the incoming data stream. Because the generated clock signal is undefined, it is useless to continue the test. You may consider using an external clock.

UDATa (Unlocked DATa, only available for the E4869B and N4872A to N4875A modules) If this value is returned, the input clock is not stable enough.

Any return value other than **LOCKed** indicates that the internal and external signals are not locked. In this case, you can do the following to identify the problem:

- Check the physical connection to the module
- Check the level parameter or the frequency of the supplied signal
The supplied signal should be roughly equal to the internal frequency of the module. You can check this in the GUI.

Example :_test:SGEN:GLOB:PLL:STAT?

might return:

LOCK

:SGENeral:GLOBal:CONFigure Subsystem

Syntax :<Handle>:SGENeral:GLOBal:CONFigure

In accordance with the SCPI standard, this subsystem is used to perform measurements. The Agilent 81250 System offers three measurement modes:

- The Capture Data mode
- The Error Rate Measurement mode
- The Compare and Acquire around Error mode

:<Handle>:SGENeral:GLOBal:CONFigure?

Syntax :<Handle>:SGENeral:GLOBal:CONFigure?

Return Value Returns the last measurement mode setting in a quoted string (“ECO FAIL”, “ECO ONES”, “ECO ZER”, “ECAP <number of stop bits>”).

Example :_test:SGEN:GLOB:CONF?

might return:

"ECO FAIL"

:<Handle>:SGENeral:GLOBal:CONFigure:CAPTURE

Syntax :<Handle>:SGENeral:GLOBal:CONFigure:CAPTURE

Description In the CAPTURE measurement mode, it is possible to hook up analyzer channels at the output or input of the DUT (Device Under Test), capture (acquire) the data stream and then use the captured data stream as stimulus data or just to see what happens.

Example :_test:SGEN:GLOB:CONF:CAPT

:<Handle>:SGENeral:GLOBal:CONFigure[: ECOut]

Syntax :<Handle>:SGENeral:GLOBal:CONFigure[:ECOut][FAILures | ONESfailed | ZERosfailed]

In the Error Rate (Error COunt) measurement mode, an expected data segment (or more) is compared and the failed bits are counted. To read the results, see “:FETCh[:ECOut]?” on page 312.

If the argument is omitted, the default mode is count all FAILures.

Example :_test:SGEN:GLOB:CONF ONES

:<Handle>:SGENeral:GLOBal:CONFigure: ECAPture

Syntax :<Handle>:SGENeral:GLOBal:CONFigure:ECAPture[<StopBits>]

Range/Value Coupling On E4832A and E4861A modules, there is no restriction for the frequency multiplier.

The frequency multiplier can be queried via CGR:MOD:CONN:MUX?

The segment resolution can be queried via SGEN:GLOB:MUX?

Description In the Error CAPture mode, the incoming data stream is compared to a stream of expected data. After compare, the resulting data stream is held in the internal memory ready to be displayed or to be saved to the database. An additional parameter can be specified called <StopBits>. This is a number of cycles that can be specified to stop the analyzer after an error occurs. If the parameters are omitted following default values are assumed: StopBits= 32768.

For systems housing E4832A or E4861A modules, the minimum number of stop bits is 976.

Note that the value is always rounded up internally because of the resolution. Note that because of clock uncertainty, a few additional bits (depending on resolution) are recorded.

Example :_test:SGEN:GLOB:CONF:ECAP 1024

:<Handle>:SGENeral:GLOBal:CONFigure:CCAPture

Syntax :<Handle>:SGENeral:GLOBal:CONFigure:CCAPture

Range/Value Coupling On E4832A and E4861A modules there is no restriction for the frequency multiplier.

The frequency multiplier can be queried via CGR:MOD:CONN:MUX?

The segment resolution can be queried via SGEN:GLOB:MUX?

Reset Value After reset the system is in the ECO mode.

Description Sets the instrument to Compare and CAPture mode. In this mode, the incoming data stream is compared to a stream of expected data. Errors can be handled via event handling, for example, a deferred branch to the sequence end.

Example :_test:SGEN:GLOB:CONF:CCAP
:_test:SGEN:GLOB:CONF?
= CCAP

:SGENeral:GLOBal:INITiate: CONTInuous Subsystem

Syntax :<Handle>:SGENeral:GLOBal:INITiate:CONTInuous

This subsystem controls the initialization of the trigger subsystem. In other words, these commands are used to start or stop the instrument (system).

:<Handle>:SGENeral:GLOBal:INITiate: CONTInuous

Syntax :<Handle>:SGENeral:GLOBal:INITiate:CONTInuous <ON | OFF>

Parameters <ON | OFF> ON starts the system.

This command starts/stops the system.

Example :_test:SGEN:GLOB:INIT:CONT ON

:<Handle>:SGENeral:GLOBal:INITiate: CONTInuous?

Syntax :<Handle>:SGENeral:GLOBal:INITiate:CONTInuous?

Return Value The current state of the system.

Example :_test:SGEN:GLOB:INIT:CONT ON
 ...
 :_test:SGEN:GLOB:INIT:CONT?
 ON
 :_test:SGEN:GLOB:INIT:CONT OFF
 ...
 :_test:SGEN:GLOB:INIT:CONT?
 OFF

:SGENeral:GLOBal:SYSTem Subsystem

Syntax :<Handle>:SGENeral:GLOBal:SYSTem

The system is started or stopped by the previous command.

It is also possible that a system is stopped for example by the actual sequence, for example, if the sequence finishes before a stop was initiated by the user.

:<Handle>:SGENeral:GLOBal:SYSTem:STATe?

Syntax :<Handle>:SGENeral:GLOBal:SYSTem:STATe?

Return Value Returns the current state of the system.

The system is started or stopped by the previous command. It is also possible that a system is stopped for example by the actual sequence, for example, if the sequence finishes before a stop was initiated by the user.

The possible return values are:

FINished	The system has finished the sequence to generate
HALTed	The system is halted due to external gate or external stop
PROGram	The system is in the programming state (all parameters can be changed)
RUNNing	The system is in the running state (a data stream is generated)
SYNChronizing	The system is currently synchronizing on the data pattern

Example :_test:SGEN:GLOB:SYST:STAT?

might return:

PROG

:SGENeral:GLOBal:SEQuence Subsystem

Syntax :<Handle>:SGENeral:GLOBal:SEQuence

This subsystem includes all commands related to sequencing. The functionality presented here is shown in the GUI as “Sequence Editor” and the “Prepare” Button.

It is recommended to use the GUI to set up and modify sequences. Afterwards, the sequence can be queried via the Command Line window. The resulting sequence or event expressions can then be integrated into remote programs via cut and paste.

Hierarchical Expressions

Sequences and Events use hierarchical expressions to encode information. The Syntax of an hierarchical expression is presented in EBNF notation (see ISO 14977):

- " or ' are quote characters, everything enclosed by quotes is treated “as is”.
- * is a repetition symbol, for example, 3 * “a” means aaa
- | separates alternative definitions
- ::= is the defining symbol
- ; ends a definition
- () groups a definition
- [] encloses optional nodes
- { } encloses repetitive rules

:<Handle>:SGENeral:GLOBal:SEQuence[:VALue]

Syntax :<Handle>:SGENeral:GLOBal:SEQuence[:VALue] <(Expression)>

Parameters <(Expression)> hierarchical expression, syntax as described below

The sequence-expression is a simple programming language, defined by the following EBNF:

```

Sequence-Expression ::= "(1.0," Label "," Block-Expression-1 ")" |
                       "(2.0," Label "," Block-Expression-2 ")" |
                       "(3.0," Label "," Block-Expression-3 )" ;
Block-Expression-1  ::= Simple-Expression-1 | Sequential-
                       Expression-1 | Loop-Expression-1 ;
Simple-Expression-1 ::= "(BLOCK," Trigger "," Vectors { ","
                       Segment } ")" ;
Sequential-Expression-1 ::= "(SEQ," Block-Expression-1 { "," Label ","
                              Block-Expression-1 } ")" ;
Loop-Expression-1    ::= "(LOOP" (1|2|3|4|5) "," Trigger ","
                              Iterations "," Block-Expression-1 )" ;
Block-Expression-2   ::= Simple-Expression-2 |
                       Sequential-Expression-2 |
                       Loop-Expression-2 ;
Simple-Expression-2  ::= "(BLOCK," Trigger "," Vectors ",0," VXI-
                       Triggers-2 "," React-Expressions-2 { ","
                       Segment )" ;
Sequential-Expression-2 ::= "(SEQ," Block-Expression-2 { "," Label ","
                              Block-Expression-2 } )" ;
Loop-Expression-2    ::= "(LOOP" (1|2|3|4|5) "," Trigger ","
                              Iterations "," VXI-Triggers-2 "," Block-
                              Expression-2 )" ;
React-Expressions-2  ::= "( React-Expression-2 { ","
                              React-Expression-2 } )" ;
React-Expression-2   ::= "(" Event-2 "," Goto-2 "," Trigger ","
                              VXI-Triggers-2 )" ;
Segment              ::= Segment-Name ",0,0" ;
Block-Expression-3   ::= Simple-Expression-3 |
                       Sequential-Expression-3 |
                       Loop-Expression-3 ;
Simple-Expression-3  ::= "(BLOCK," Trigger "," Vectors ",0,"
                       VXI-Triggers-2 ","
                       React-Expressions-3 { "," Segment } )" ;

```

```

Sequential-Expression-3 ::= "(SEQ," Block-Expression-3 { "," Label ",
                          "Block-Expression-3 } )";
Loop-Expression-3      ::= "(LOOP" (1|2|3|4|5) "," Trigger ","
                          Iterations "," VXI-Triggers-2 ","
                          Block-Expression-3 )";
React-Expressions-3   ::= React-Expressions-2 | Sync-Expression-
                          3;
Sync-Expression-3     ::= "SYNC";
Segment-Name          ::= String | "PAUSE0" | "PAUSE1" |
                          "ACQUIRE" | "PAUSE" | "EXPECTED0" |
                          "EXPECTED1" | "PAUSE" |
                          "EXPECTED0" | "EXPECTED1" |
                          "DONTCARE" | "PAUSE" ;
Label                 ::= String ;
Trigger               ::= "0" | "1" ;
Vectors               ::= Number ;
Iterations             ::= Number | "INF" ;
VXI-Triggers-2       ::= "" 2 * ( "0" | "1" ) "" |
                          "" 2 * ( "0" | "1" ) "" ;
Event-2               ::= String ;
Goto-2                ::= String ;
Number                ::= { Digit } ;
Digit                 ::= "0" | "1" | "2" | "3" | "4" | "5" | "6" | "7" |
                          "8" | "9" ;
String                ::= "" [ Letter { Letter | Digit } ] "" |
                          "" [ Letter { Letter | Digit } ] "" ;
Letter                ::= "_" | "A" | "B" | "C" | "D" | "E" | "F" | "G"
                          | "H" | "I" | "J" | "K" | "L" | "M" | "N" | "O"
                          | "P" | "Q" | "R" | "S" | "T" | "U" | "V" |
                          "W" | "X" | "Y" | "Z" | "a" | "b" | "c" | "d" |
                          "e" | "f" | "g" | "h" | "i" | "j" | "k" | "l" | "m"
                          | "n" | "o" | "p" | "q" | "r" | "s" | "t" | "u" |
                          "v" | "w" | "x" | "y" | "z" ;

```

NOTE It is recommended to set up sequences in the graphical user interface. The resulting sequence expression can then be queried in the Command Line window. Afterwards, the sequence expression can easily be used in your program editor by copy and paste.

Range/Value Coupling Event-2 names are defined by the events-expression described in the command. The expression is stored and checked against the number of ports and the maximum number of segments.

The expression is evaluated under two conditions:

- An SGEN:GLOB:SEQ:FORC command is executed.
- An SGEN:GLOB:INIT:CONT ON command is executed and the sequence expression is changed, or another parameter is changed that requires a new sequence / data download.

Therefore, syntax errors within the expression or range violations are detected only after these conditions.

Adding or removing ports changes the number of “Segment” entries needed. Therefore the sequence expression is automatically adjusted by inserting and deleting “Segment” entries. Inserted “Segment” entries depend on the port type:

- For INPUT_PORTS, an entry with a PAUSE0 segment is inserted.
- For OUTPUT_PORTS, an entry with a PAUSE segment is inserted.

The number of vectors depends on the system Segment Resolution as specified by the SGEN:GLOB:MUX command. The number of vectors must be a multiple of the Segment Resolution value. The minimum value depends on the number of looping levels started on that block: It must be $(1 + \text{“Number of Looping Levels Started”}) * \text{“Segment Resolution”}$.

The sequence will be downloaded with the next SGEN:GLOB:INIT:CONT ON command when one of the following happens:

- The channel add configuration changed (...:OUTP:CAC).
- A data port is added or deleted (SGEN:PDAT:APP, SGEN:PDAT(*):REM).
- A terminal within a data port is added or deleted (SGEN:CONN:PDAT(*):TERM, SGEN:CONN:PDAT(*):REM).
- The formatter mode is changed (...:DIG:STIM:SIGN:FORM).
- A frequency multiply factor is changed (...:MUX).
- The Segment Resolution is changed (SGEN:GLOB:MUX).
- A segment is changed (via the EDIT subsystem or via segment import MMEM:SEGM:LOAD).

Limits Vectors Just limited by the memory of the modules.

Iterations Up to 2^{20} or infinite on the highest available looping level (2 or 5 depending on the clock module used (see “:<Handle>:SGENeral:GLOBal:SEQuence:LLEVel?” on page 165).


Segment-Name Valid keywords, depending on the port type and measurement mode:

- Output Port: PAUSE0 and PAUSE1
- Input Port, Capture: ACQUIRE and PAUSE
- Input Port, Bit Error Rate: EXPECTED0, EXPECTED1, PAUSE
- Input Port, Compare and Acquire around Error: EXPECTED0, EXPECTED1, DONTCARE and PAUSE.

Description With this command, the data sequence is loaded into the system. The sequence expression corresponds to the Sequence Editor of the graphical user interface.

Example `:_test:SGEN:GLOB:SEQ (1.0,"", (SEQ, (BLOCK,0,80, "header",0,0, PAUSE, 0, 0),"", (LOOP5,0,INF, (BLOCK,0,80, "count16up",0,0,"count16up",0,0))))`

results in the following sequence, as shown in the graphical user interface:

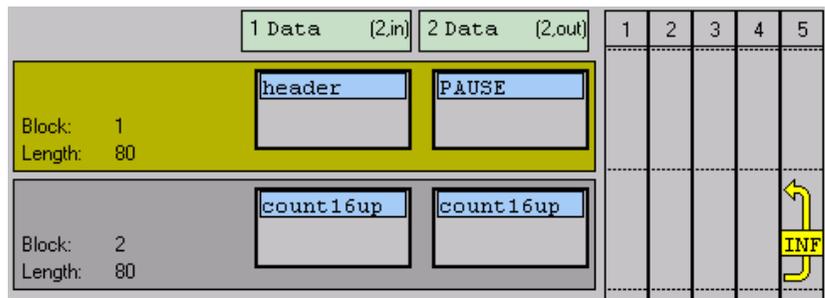

:<Handle>:SGENeral:GLOBal:SEQuence[:VALue]?

Syntax :<Handle>:SGENeral:GLOBal:SEQuence[:VALue]?

Return Value This query returns the current data sequence of the system.

Example :_test:SGEN:GLOB:SEQ?

might return:

```
(1.0, "", (SEQ, (BLOCK, 0, 80, "header", 0, 0, PAUSE, 0, 0), "",  
(LOOP5, 0, INF, (BLOCK, 0, 80, "count16up", 0, 0, "count16up", 0, 0))))
```

:<Handle>:SGENeral:GLOBal:SEQuence:EVENTs

Syntax :<Handle>:SGENeral:GLOBal:SEQuence:EVENTs <event-expression>

Parameters <event-expression> hierarchical expression, syntax described below

The event expression is a simple programming language, defined by the following EBNF:

```

Events-Expression ::= "(2.0," 10 * Event-Expression ")" |
                    "(3.0," 10 * Event-Expression)";
Event-Expression  ::= "(" Name "," Enabled "," Or-Expressions)";
Or-Expressions    ::= "(" Or-Expression { "," Or-Expressions })";
Or-Expression     ::= "(" CMD "," POD "," VXI-Triggers "," Errors)";
                    ;
Name              ::= String ;
Enabled           ::= "0" | "1" ;
CMD               ::= "" 1 * Bit-Mask "" | "" 1 * Bit-Mask "" ;
POD               ::= "" 8 * Bit-Mask "" | "" 8 * Bit-Mask "" ;
VXI-Triggers      ::= "" 2 * Bit-Mask "" | "" 2 * Bit-Mask "" ;
Errors            ::= "IGNORE" | "ERROR" | "NOERROR" |
                    "ERROR" Number | "NOERROR" Number ;
Bit-Mask          ::= "0" | "1" | "x" | "X" ;
Number            ::= { Digit } ;
Digit             ::= "0" | "1" | "2" | "3" | "4" | "5" | "6" | "7" | "8" |
                    "9" ;
String            ::= "" Letter { Letter | Digit } "" | "" Letter {
                    Letter | Digit } "" ;
Letter            ::= "_" | "A" | "B" | "C" | "D" | "E" | "F" | "G" | "H"
                    | "I" | "J" | "K" | "L" | "M" | "N" | "O" | "P" |
                    "Q" | "R" | "S" | "T" | "U" | "V" | "W" | "X" | "Y"
                    | "Z" | "a" | "b" | "c" | "d" | "e" | "f" | "g" | "h" |
                    "i" | "j" | "k" | "l" | "m" | "n" | "o" | "p" | "q" |
                    "r" | "s" | "t" | "u" | "v" | "w" | "x" | "y" | "z" ;

```

Range/Value Coupling The events defined here are used by the sequence expression.

The expression is just stored and not checked. The expression is evaluated under two conditions:

- An SGEN:GLOB:SEQ:FORC command is executed.
- An SGEN:GLOB:INIT:CONT ON command is executed and the sequence expression is changed, or another parameter is changed that requires a new sequence / data download.

Therefore, syntax errors within the expression or range violations are detected only after these conditions.

The values possible for the Error events depend on the receive mode used. In Capture Mode the error events are simply ignored.

Deleting a port results in an error event (invalid port). Therefore, the event-expression is automatically adjusted to remove this error event.

Reset Value As reset value all 10 events are disabled:

```
(3.0, (,0, (('x', 'xxxxxxxx', 'xx', IGNORE))),
(,0, (('x', 'xxxxxxxx', 'xx', IGNORE)))
```

Limits The specified events must be unique. The events to be used must be unambiguous.

Description: With this command the events are defined for the system. The event expression corresponds to the Event Editor of the graphical user interface.

Example `sgen:glob:seq:even (2.0, (,0, (('x', 'xxxxxxxx', 'xx', IGNORE))),`
`(,0, (('x', 'xxxxxxxx', 'xx', IGNORE)))`

:<Handle>:SGENeral:GLOBal:SEQuence:EVENTs?

Syntax :<Handle>:SGENeral:GLOBal:SEQuence:EVENTs?

Range/Value Coupling: This query is only available for E4805B and E4808A clock modules. The events defined here are used by the sequence expression.

Reset Value (2.0, (, 0, (('x', 'xxxxxxxx', 'xx', IGNORE))),
 (, 0, (('x', 'xxxxxxxx', 'xx', IGNORE)))

Description This query returns the events defined by the system. The event-expression corresponds to the Event Editor of the graphical user interface.

Example SGEN:GLOB:SEQ:EVEN?
 might return:

```
(2.0, (, 0, (('x', 'xxxxxxxx', 'xx', IGNORE))),  

  (, 0, (('x', 'xxxxxxxx', 'xx', IGNORE)))
```

:<Handle>:SGENeral:GLOBal:SEQuence:FORCe

Syntax :<Handle>:SGENeral:GLOBal:SEQuence:FORCe

Description Downloads the sequence (including events and data) into the hardware. The command corresponds to the *Prepare* button in the graphical user interface.

This command is useful when you want a fixed execution time for the SGEN:GLOB:INIT:CONT ON command. Otherwise, the SGEN:GLOB:INIT:CONT ON command downloads the sequence as needed and may therefore have different execution times depending on the history of commands that have been sent to the system.

Example :_test:SGEN:GLOB:SEQ:FORC

:<Handle>:SGENeral:GLOBal:SEQuence:LLEVel?

Syntax :<Handle>:SGENeral:GLOBal:SEQuence:LLEVel?

Return Value Returns the actual number of available looping levels.

The graphical user interface uses this command to offer 5 looping levels in the Sequence Editor.

Example :_test:SGEN:GLOB:SEQ:LLEV?

might return:

5

:<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol

Syntax	:<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol <Nrf>
Parameters	Value in Nrf format.
Range/Value Coupling	May influence the data sequence at runtime.
Reset Value	0
Limits	Valid values are 0 and 1.
Description	Sets the value of the program control event. With this event, which is part of the events defined by the events-expression, the data sequence can be influenced at runtime. This may be used for “Stop and Go” sequence model, etc.
Example	SGEN:GLOB:SEQ:PCON 1

:<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol?

Syntax	:<Handle>:SGENeral:GLOBal:SEQuence:PCONtrol?
Reset Value	0
Description	Returns the state of the program control event line.
Example	SGEN:GLOB:SEQ:PCON? might return: 1

:<Handle>:SGENeral:GLOBal:SEQuence:STATe?

Syntax	:<Handle>:SGENeral:GLOBal:SEQuence:STATe?
Description	The sequence indicator returns the number of the currently executed block. If “0” is returned, the system is stopped or none of the modules in the system supports the sequence indicator. The sequence indicator is supported by the modules 3.3G, 7G and 13G.

Example :SGEN:GLOB:SEQ:STAT?

might return:

1 (the first block is currently executed)

:SGENeral:GLOBal:SYNChronization Subsystem

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization

This command system includes:

- Commands and queries for setting up the automatic alignment of incoming and expected data.
- DeMUX rewiring commands.

The following figure shows the DeMUX rewiring commands in the Agilent 81250 user interface.

:SGEN:PDAT:DMUX:STAG1 :SGEN:GLOB:SYNC:APS :SGEN:GLOB:SYNC:BER :SGEN:GLOB:SYNC:PACC

:SGEN:GLOB:SYNC:SMOD BSYN
:SGEN:GLOB:SYNC:SMOD FBSY
:SGEN:GLOB:SYNC:SMOD DAL

:SGEN:GLOB:SYNC:REW ON
:SGEN:GLOB:SYNC:REW OFF

:SGEN:GLOB:SYNC:RMOD AUTO
:SGEN:GLOB:SYNC:RMOD TRO
:SGEN:GLOB:SYNC:RMOD TDET

:SGEN:GLOB:SYNC:RCH ON
:SGEN:GLOB:SYNC:RCH OFF

:SGEN:PDAT:DMUX:STAG1:OUT 16

For the description of the DeMUX rewiring parameter commands, see “*DeMUX Rewiring Parameter Commands*” on page 217.

:<Handle>:SGENeral:GLOBal:SYNChronization:USED?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:USED?

Return Value The query can only succeed (return TRUE) when there is at least one analyzer capable of synchronization installed.

Returns TRUE if the synchronization flag is found somewhere in the sequence and at least one analyzer capable of synchronization is installed.

Returns FALSE otherwise.

Example :_test:SGEN:GLOB:SYNC:USED?
 might return:
 TRUE

:<Handle>:SGENeral:GLOBal:SYNChronization:BERThreshold

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:BERThreshold <Thresh>

Parameters <Thresh> Threshold for the bit error ratio to be accepted during synchronization. The range is from 1e-4 to 1e-9. The reset value is 1e-6.

Note that the time needed for synchronization increases with decreasing bit error ratio threshold. To assure that the bit error ratio is lower than the threshold, $N * 1/\langle\text{Thresh}\rangle$ bits must be measured ($N > 1$).

<Thresh> is used during the synchronization process to determine whether the synchronization was successful. If after an internal synchronization attempt the bit error ratio is larger than this value, a new synchronization will be started. The synchronization block is only left when the bit error ratio is below the <Thresh> value.

This value is also used to calculate the optimum sampling point during sampling point optimization (phase adjust).

Note that this value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE.

Example :_test:SGEN:GLOB:SYNC:BERT 1e-9

:<Handle>:SGENeral:GLOBal: SYNChronization:BERTHreshold?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:BERTHreshold?

Return Value Returns the programmed bit error ratio threshold. Note that this value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE.

Example :_test:SGEN:GLOB:SYNC:BERT?

might return:

1e-9

:<Handle>:SGENeral:GLOBal: SYNChronization:SMODE

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:SMODE <BSYNchronization | DALignment | FBSYNchronisation>

Parameters Specifies how the synchronization of the analyzers is achieved. Note that this value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE.

BSYNchronization Neither the exact delay nor a delay range is known within which the incoming data will start. The data can come at any time after the system is started. The actual delay will be determined by automatic bit synchronization.

This is the reset value.

DALignment The exact sample delay is not known in advance, but a certain delay range the correct sample point will be inside. The actual delay will be determined by automatic delay adjustment.

FBSYNchronisation A method for aligning expected PRBS or PRWS data with incoming data very quickly. This method does not change the analyzer sampling delay.

Example :_test:SGEN:GLOB:SYNC:SMOD BSYN

:<Handle>:SGENeral:GLOBal:SYNChronization:SMODE?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:SMODE?

Return Value Returns the currently set synchronization mode.

Note that this value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE.

Example :_test:SGEN:GLOB:SYNC:SMOD?

might return:

BSYN

:<Handle>:SGENeral:GLOBal:SYNChronization:APSelect

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:APSelect TRUE|FALS

Description Enables/disables the **Automatic Polarity Select** feature. When this feature is enabled, the synchronizing analyzer channel will first try to synchronize the incoming signal with the currently selected input polarity. If this fails, it will try to synchronize with the opposite input polarity.

This feature is only available if all analyzer channels in the system are able to select the input polarity. Currently, this is only supported by:

- E4832A (E4835A frontend) modules
- E4861B (E4863B frontend) modules
- E4811A modules
- N4873/75A modules

NOTE It is not supported by the E4861A.

The input polarity after the synchronization can be queried using the query “:INPut:POLarity?” on page 246. The input polarity is also displayed in the corresponding property windows.

Example :_test:SGEN:GLOB:SYNC:APS FALS

:<Handle>:SGENeral:GLOBal:SYNChronization:APSelect?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:APSelect?

Return Value Returns whether the Automatic Polarity Select feature is enabled or disabled. Use “:INPut:POLarity?” on page 246 to query the signal’s polarity.

Example :_test:SGEN:GLOB:SYNC:APS?

might return:

TRUE

:<Handle>:SGENeral:GLOBal:SYNChronization:APAlignment

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:APAlignment <FALSe | TRUE>

Parameters Specifies whether a phase optimization is done after an automatic bit synchronization.

TRUE The phase is automatically optimized as specified by the SGEN:GLOB:SYNC:BERT and SGEN:GLOB:SYNC:PACC commands.

This is the reset value.

FALSe No automatic phase alignment.

Note that this value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE and SGEN:GLOB:SYNC:SMOD? returns BSYN.

Example SGEN:GLOB:SYNC:APA TRUE

:<Handle>:SGENeral:GLOBal:SYNChronization:APAligment?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:APAligment?

Return Value Returns TRUE or FALSE depending on whether phase optimization will be performed after an automatic bit synchronization.

Note that this value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE and SGEN:GLOB:SYNC:SMOD? returns BSYN.

Example SGEN:GLOB:SYNC:APA?
might return:
TRUE

:<Handle>:SGENeral:GLOBal:SYNChronization:PACCuracy

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:PACCuracy <accuracy>

Parameters <accuracy> Specifies in percent of the data period how accurate the phase optimization is done after a synchronization. Note that the time needed to achieve synchronization increases with the accuracy.

The range is from 0.01 to 0.2. The reset value is 0.2 (20 %).

Note that this value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE.

Example SGEN:GLOB:SYNC:PACC 0.01

:<Handle>:SGENeral:GLOBal:SYNChronization:PACCuracy?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronization:PACCuracy?

Return Value Returns the currently programmed phase accuracy to be achieved by automatic phase optimization after a synchronization.

This value will only be used if SGEN:GLOB:SYNC:USED? returns TRUE.

Example SGEN:GLOB:SYNC:PACC?
might return:
2E-1

:SGENeral:GLOBal:TRIGger Subsystem

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]

This command subsystem is used to set and measure the clock and clock reference.

:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]
<CDR | INT10 | VXI10 | EXT1 | EXT2 | EXT5 | EXT10 | EXTernal | EXTDirect>

Description This command sets the clock/reference or the external clock mode. The arguments available are:

CDR	Clock Data Recovery (only available for E4809A)
INT10 reference	internal clock source, 10 MHz internal clock reference
VXI10 reference	internal clock source, 10 MHz VXI backplane reference
EXT1 reference	internal clock source, 1 MHz external clock reference
EXT2 reference	internal clock source, 2 MHz external clock reference
EXT5 reference	internal clock source, 5 MHz external clock reference
EXT10 reference	internal clock source, 10 MHz external clock reference
EXTernal	external clock source
EXTernal Direct	external clock source direct, not handled by ParBERT

For more information on clock sources, please refer to the *Agilent 81250 Parallel Bit Error Ratio Tester System User Guide*.

NOTE If the external clock mode is set and the external start mode is selected, the external clock must be in a stable state for 100 ms before the external start can take place.

Example :_test:SGEN:GLOB:TRIG EXT5

:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]?

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]?

Return Value This query returns the actual status of the clock/reference input of the central clock module. For possible values, see “:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]” on page 173.

Example :_test:SGEN:GLOB:TRIG?

might return:

EXT5

:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDRList?

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDRList?

Return Value Returns the list of channels that have CDR (Clock Data Recovery) capabilities.

Example :_test:SGEN:GLOB:TRIG:CDRL?

might return:

= (@0104001,0103001)

:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDR

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDR<channel>

Description Specifies which channel recovers the clock from the data stream (while operating in CDR mode). CDR mode is set using “:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]” on page 173.

Parameters <channel> Defines the channel in the form “GGMMCCC”, where GG is the clockgroup, MM the module and CCC the channel number.

Example :_test:SGEN:GLOB:TRIG CDR
:_test:SGEN:GLOB:TRIG:CDR "0103001"

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQuence][:LAYer][:SOURce]:CDR?

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]:CDR?

Return Value Returns the channel currently operating in CDR mode. The channel is returned in the form “GGMMCCC”, where GG is the clockgroup, MM the module and CCC the channel number.

Example :_test:SGEN:GLOB:TRIG:CDR?

might return:

"0103001"

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQuence][:LAYer]:CLOCK[:VALue]?

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK[:VALue]?

Return Value Measures the supplied external clock at the clock/reference input of a clock module and returns the value without changing the mode of the machine.

The external clock can only be measured when the Agilent 81250 has been stopped.

Example :_test:SGEN:GLOB:TRIG:SEQ:CLOC?

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQuence][:LAYer]:CLOCK:MEASurement[: DIRect]

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MEASurement[:DIRect]

Description This command measures the external clock and sets the corresponding mode. It is only valid for the E4809A clock module, and only has an effect if an external clock source is connected to the clock module.

If the [:DIRect] node is included with the command, it sets the mode to *External Clock Source (direct)*. Otherwise, it sets the mode to *External Clock Source*.

Example `:_test:SGEN:GLOB:TRIG:CLOC:MEAS:DIR`
 or
`:_test:SGEN:GLOB:TRIG:CLOC:MEAS`

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQuence][:LAYer]:CLOCK:MULTIplier

Syntax `:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:MULTIplier
<Multiplier>`

Parameter **<Multiplier>** Sets the clock multiplication factor in a range of 1 ...
256.

This command works only when the Agilent 81250 has been stopped.

Example `:_test:SGEN:GLOB:TRIG:CLOC:MULT 10`

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQuence][:LAYer]:CLOCK:MULTIplier?

Syntax `:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:
MULTIplier?`

Return Value Returns the current clock multiplication factor.
This command works only when the Agilent 81250 has been stopped.

Example `:_test:SGEN:GLOB:TRIG:CLOC:MULT?`
 might return:
 10

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQuence][:LAYer]:CLOCK:DIVider

Syntax `:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer]:CLOCK:DIVider
<DIVider>`

Parameters **<DIVider>** The clock divider.

Range/Value Coupling Period, frequency, measured value.

Reset Value 1

Limits Works only on a stopped machine, range from 1 ... 256.

Example `_TEST:SGEN:GLOB:TRIG:CLOC:DIV 2`

:<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:CLOCK:DIVider?

Syntax `:<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:CLOCK:DIVider?`

Queries the current clock divider.

Example `:_test:sgen:glob:trig:cloc:div?`

might return:

1

:<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:RCLock:DETECT

Syntax `:<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:RCLock:DETECT [ONCE]`

This command measures the external clock reference and sets the corresponding mode automatically. The automatically set modes are:

EXT1 reference	internal clock source with 1 MHz external clock
EXT2 reference	internal clock source with 2 MHz external clock
EXT5 reference	internal clock source with 5 MHz external clock
EXT10 reference	internal clock source with 10 MHz external clock

The E4809A can only use the EXT10 mode. The E4805B and E4808A can use all modes.

Example `:_test:SGEN:GLOB:TRIG:RCL:DET`

:<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:CLOCK:MEASurement

Syntax `:<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:CLOCK:MEASurement`

This command measures the external clock and sets the corresponding mode EXTERNAL automatically.

NOTE The commands :RCL:DET and :CLOC:MEAS cannot be executed when the system is in the running state.

Example :_test:SGEN:GLOB:TRIG:CLOC:MEAS

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQUence][:LAYer]:TVOLTage

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:TVOLTage
<TermVoltage>

Parameters <TermVoltage> Specifies the termination voltage of the clock/ref input. The available termination voltage range is -2.10 V to +3.30 V. Default is 0 V.

Example :_test:SGEN:GLOB:TRIG:TVOL 1

:<Handle>:SGENeral:GLOBal:TRIGger[: SEQUence][:LAYer]:TVOLTage?

Syntax :<Handle>:SGENeral:GLOBal:TRIGger[:SEQUence][:LAYer]:TVOLTage?

Return Value Returns the actual setting of the termination voltage of the clock/ref input.

Example :_test:SGEN:GLOB:TRIG:TVOL?

might return:

1.000000E+000

:SGENeral:GLOBal:ARM Subsystem

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEquence][:LAYer]


This command subsystem is used to control the system by an external signal.

The EXTERNAL :INPut connector at the front panel of the clock module is used to start the system by a so-called GATE or by a TRIGGER signal.


Following modes are available:

...:SOUR:IMM A pulse stream (sequence) is generated immediately as soon as the system is started by the start command.


...:SOUR:GATED A pulse stream (sequence) is generated as soon as the level at the external input connector exceeds the input threshold. A sequence can be generated by a positive or a by a negative input signal depending on the parameter set.

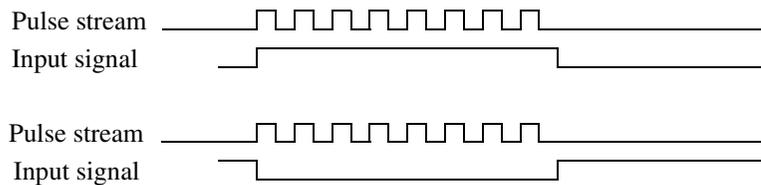

...:SOUR:STARTsignal A pulse stream (sequence) is generated as soon as a start signal exceeds the input threshold. A sequence can be started by a positive or a negative input signal depending on the parameter set.

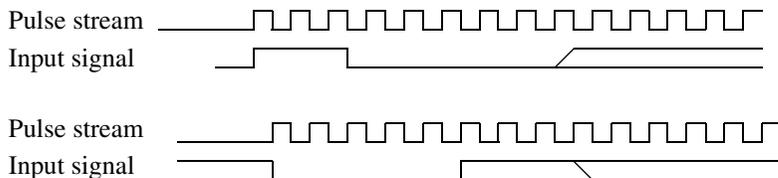

...:SOUR:STOPsignal The pulse stream (sequence) is stopped as soon as a stop signal exceeds the input threshold. The sequence can be stopped by a positive or negative input signal depending on the parameter set. All these modes are active if the system is started manually or started by a remote command.

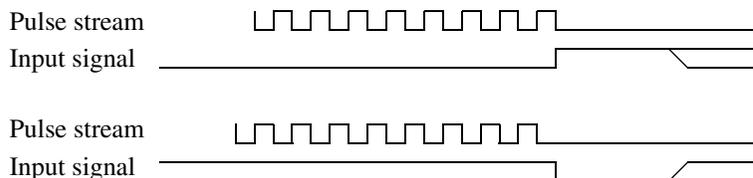

NOTE IMMEDIATE and START are always supported, GATED and STOP are only supported for E4832A modules.

:<Handle>:SGENeral:GLOBal:ARM[:SEQUENCE][:LAYER][:SOURCE]

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEQUENCE][:LAYER][:SOURCE] IMMEDIATE | GATED | STARTsignal | STOPsignal

Description This command controls the start mode of the Agilent 81250 System. If IMMEDIATE is selected, then the sequence can be started and stopped by the :SGEN:GLOB:INIT:CONT ON | OFF command, or it is possible to press the start or stop button in the graphical user interface.

NOTE If the external clock mode is set and the external start mode is selected, the external clock must be in a stable state for 100 ms before the external start can take place.

Example :_test:SGEN:GLOB:ARM IMM

:<Handle>:SGENeral:GLOBal:ARM?

Syntax :<Handle>:SGENeral:GLOBal:ARM?

Return Value This command returns the actual status of the External Input connector at the front of the central clock module. It shows how this input controls the system.

IMM Immediate

GAT Gated

STAR Started by a start signal

STOP Stopped by a stop signal

:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:SENSe

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:SENSe PLEVel | NLEVel

This command specifies the input level condition which is used in the GATed | STARtsignal | STOPsignal modes.

Example :_test:SGEN:GLOB:ARM:SENS PLEV

:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:SENSe?

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:SENSe?

Returns the actual setting of the input level condition for the gate or start/stop signal (PLEVel or NLEVel).

Example :_test:SGEN:GLOB:ARM:SENS?

might return:

PLEV

:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:THReshold

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:THReshold <NRf>

This command specifies the threshold of the external input signal which is used in the GATED | STARTsignal | STOPsignal modes. The range is from -1.40 V to +3.70 V.

Example :_test:SGEN:GLOB:ARM:THR 1

:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:THReshold?

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:THReshold?

Returns the threshold for the external input signal used in the gate or start/stop mode.

Example :_test:SGEN:GLOB:ARM:THR?

might return:

1.000000E+000

:<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:TVOLTage

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:TVOLTage <NRf>

This command specifies the termination voltage of the external input signal which is used in the GATED | STARTsignal | STOPsignal modes. The range is from -2.10 V to +3.30 V.

Example :_test:SGEN:GLOB:ARM:TVOL -2

:<Handle>:SGENeral:GLOBal:ARM[: SEQUence][:LAYer]:TVOLTage?

Syntax :<Handle>:SGENeral:GLOBal:ARM[:SEQUence][:LAYer]:TVOLTage?

Returns the actual termination voltage for the external input signal used in the gate or start/stop mode.


Example :_test:SGEN:GLOB:ARM:TVOL?

might return:

-2.000000E+000

Timing Parameter Commands

The commands for specifying the timing parameters are available on port, terminal and connector level. The parameters can be specified separately for pulse and data ports.

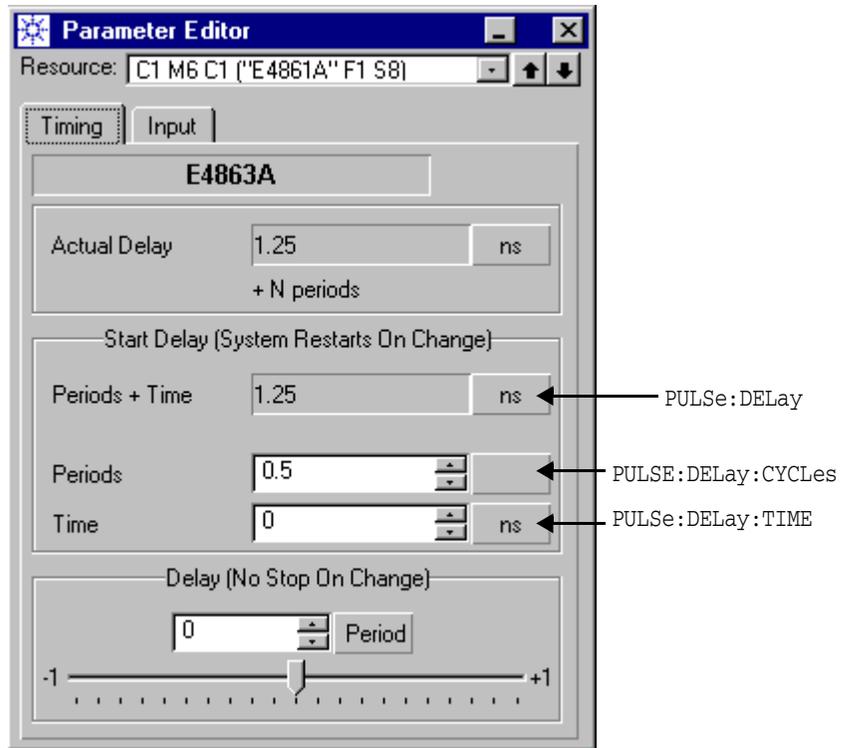

:PULSe:DELaY

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:DELaY <Delay>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:DELaY <Delay>
 :<Handle>:SGENeral:PPULse(*):[:SOURce]:PULSe:DELaY <Delay>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:PULSe:DELaY <Delay>
 :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):[:SOURce]:PULSe:DELaY <Delay>

Parameters <Delay> Delay value in seconds (<NRf>).

Description Sets the time from the start of the period to the first edge of the pulse. Reference is the trigger output.

Valid range for E4832A: 0 ... max (3 μ s, PERiod).

Valid range for E4861A, E4866A: 0 ... 300 ns.

Valid range for E4861B: 0 ... 200 ns.

Valid range for N4872A/N4874A: 0 ... 200 ns.

If this command is used, the value is interpreted as a timing value only. This sets PULSe:DELaY:CYCLes to zero.

Otherwise, if the delay is specified by PULSe:DELaY:CYCLes and PULSe:DELaY:TIME, the corresponding delay is calculated. The number of cycles is converted into seconds and added to the specified PULSe:DELaY:TIME value.

Example :_test:SGEN:PDAT1:PULS:DEL 50e-9
 :_test:SGEN1:PDAT1:TERM1:PULS:DEL 50e-9
 :_test:SGEN:PDAT1:PULS:DEL 50e-9
 :_test:SGEN1:PDAT1:TERM1:PULS:DEL 50e-9
 :_test:CGROUP1:MODULE2:CONNECTOR4:PULS:DEL 50e-9

:PULSe:DElAy?

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:DElAy?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:DElAy?
 :<Handle>:SGENeral:PPULs(*):[:SOURce]:PULSe:DElAy?
 :<Handle>:SGENeral:PPULs (*):TERMinal(*):[:SOURce]:PULSe:DElAy?
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):[:SOURce]:PULSe:DElAy?

Return Value Returns the current pulse delay value.

Example :_test:SGEN:PDAT1:PULS:DEL?
 :_test:SGEN1:PDAT1:TERM1:PULS:DEL?
 :_test:SGEN:PPUL1:PULS:DEL?
 :_test:SGEN1:PPUL1:TERM1:PULS:DEL?
 :_test:CGROUP1:MODULE2:CONNECTOR4:PULS:DEL?
 might return:
 5.000000E-008

:PULSe:DElAy:CYCLes

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:DElAy:CYCLes <Cycles>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:DElAy:
 CYCLes <Cycles>
 :<Handle>:SGENeral:PPULs(*):[:SOURce]:PULSe:DElAy:CYCLes <Cycles>
 :<Handle>:SGENeral:PPULs (*):TERMinal(*):[:SOURce]:PULSe:DElAy:
 CYCLes <Cycles>
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):[:SOURce]:PULSe:DElAy:
 CYCLes <Cycles>

Parameters **<Cycles>** One cycle corresponds to the actual period/frequency valid for the specified generator output connector.

If the delay is specified by DElAy:CYCLes and PULSe:DElAy:TIME, the corresponding delay will be calculated. The number of cycles is converted into seconds and added to the specified PULSe:DElAy:TIME value.

If PULSe:DElAy is used, the value is interpreted as a timing value only. This sets PULSe:DElAy:CYCLes to zero.

Example : _test:SGEN:PDAT1:PULS:DEL:CYCL 0.5
 : _test:SGEN1:PDAT1:TERM1:PULS:DELAY:CYCL 0.5
 : _test:SGEN:PPUL1:PULS:DEL:CYCL 0.5
 : _test:SGEN1:PPUL1:TERM1:PULS:DELAY:CYCL 0.5
 : _test:CGROUP1:MODULE2:CONNECTOR4:PULS:DELAY:CYCL 0.5

:PULSe:DELay:CYCLes?

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:DELay:CYCLes?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:DELay:
 :CYCLes?
 :<Handle>:SGENeral:PPULs(*):[:SOURce]:PULSe:DELay:CYCLes?
 :<Handle>:SGENeral:PPULs (*):TERMinal(*):[:SOURce]:PULSe:DELay:
 CYCLes?
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNector(*):[:SOURce]:PULSe:DELay:
 :CYCLes?

Return Value Returns the current cycle value of the pulse delay for the specified generator output connector.

Example : _test:SGEN:PDAT1:PULS:DEL:CYCL?
 : _test:SGEN1:PDAT1:TERM1:PULS:DEL:CYCL?
 : _test:SGEN:PPUL1:PULS:DEL:CYCL?
 : _test:SGEN1:PPUL1:TERM1:PULS:DEL:CYCL?
 : _test:CGROUP1:MODULE2:CONNECTOR4:PULSE:DELAY:CYCL?

might return:

5.000000E-001

:PULSe:DELay:TIME

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:DELay:TIME <Time>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:DELay:TIME <Time>
 :<Handle>:SGENeral:PPULs(*):[:SOURce]:PULSe:DELay:TIME <Time>
 :<Handle>:SGENeral:PPULs (*):TERMinal(*):[:SOURce]:PULSe:DELay:TIME <Time>
 :<Handle>[:CGROUP(*):MODULE(*):CONNECTor(*):[:SOURce]:PULSe:DELay:TIME <Time>

Parameters <Time> Delay in seconds.

If the delay is specified by DELay:TIME and PULSe:DELay:TIME, the corresponding delay is calculated. The number of cycles is converted into seconds and added to the specified PULSe:DELay:TIME value.

If PULSe:DELay is used, the value is interpreted as a timing value only. This sets PULSe:DELay:TIME to zero.

Example :_test:SGEN:PDAT1:PULS:DEL:TIME 0.5
 :_test:SGEN1:PDAT1:TERM1:PULS:DEL:TIME 0.5
 :_test:SGEN:PPUL1:PULS:DELAY:TIME 0.5
 :_test:CGROUP1:MODULE2:CONNECTOR4:PULS:DELAY:TIME 0.5

:PULSe:DELay:TIME?

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:DELay:TIME?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:DELay:TIME?
 :<Handle>:SGENeral:PPULs(*):[:SOURce]:PULSe:DELay:TIME?
 :<Handle>:SGENeral:PPULs (*):TERMinal(*):[:SOURce]:PULSe:DELay:TIME?
 :<Handle>[:CGROUP(*):MODULE(*):CONNECTor(*):[:SOURce]:PULSe:DELay:TIME?

Return Value Returns the current cycle value of the pulse delay for the specified generator output connector.

Example :_test:SGEN:PDAT1:PULS:DELAY:TIME?
 :_test:SGEN1:PDAT1:TERM1:PULS:DEL:TIME?
 :_test:SGEN:PPUL1:PULS:DEL:TIME?
 :_test:CGROUP1:MODULE2:CONNECTOR4:PULSE:DELAY:TIME?

might return:

5.000000E-001

:PULSe:CROSSing

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:CROSSing <CROSSing>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:CROSSing
 <CROSSing>
 :<Handle>:SGENeral:PPULse(*):[:SOURce]:PULSe:CROSSing <CROSSing>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:PULSe:CROSSing
 <CROSSing>
 :<Handle>[:CGRoup(*):MODUle(*):CONNector(*):[:SOURce]:PULSe:CROSSing
 <CROSSing>

Parameters <CROSSing> Cross point of the signal in percentage of signal amplitude. The formula for the cross point is:

$$\text{Cross Point} = 100 * ((V_{\text{Cross}} - V_{\text{High}}) / (V_{\text{High}} - V_{\text{Low}}))$$

This parameter is valid only for NRZ format modes.

Cross point range is subject to change; depending on hardware capabilities.

Valid range for E4862B: 25 ... 75 %

Valid range for N4872A/74A: 20 ... 80 %

NOTE This parameter can also be used for the N4868A 10.8G Booster modules. The valid range is: 40 ... 60 %

Example :_test:SGEN:PDAT1:PULS:CROS 40.0
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:CROS 40.0
 :_test:SGEN:PPUL1:PULS:CROS 40
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:CROS 40
 :_test:MODULE2:CONNECTOR3:PULSE:CROSSING 40.0

:PULSe:CROSSing?

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:CROSSing?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:CROSSing?
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:CROSSing?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:CROSSing?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:CROSSing?

Return Value Returns the current cross point. The unit for the cross point is in percentage of signal amplitude. The formula for the cross point is:

$$\text{Cross Point} = 100 * ((V_{\text{Cross}} - V_{\text{High}}) / (V_{\text{High}} - V_{\text{Low}}))$$

Example :_test:SGEN:PDAT1:PULS:CROS?
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:CROS?
 :_test:SGEN:PPUL1:PULS:CROS?
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:CROS?
 :_test:MODULE2:CONNECTOR3:PULSE:CROSSING?

might return:

50.0

:PULSe:WIDTh

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:WIDTh <Width>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:WIDTh <Width>
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:WIDTh <Width>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:WIDTh <Width>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:WIDTh <Width>

Parameters <Width> Pulse width in seconds (<Nrf>).

Sets the width or duration of the pulse.

Valid range 0 ... PERiod

(on connector level: 0 ... PERiod / Connector:MUX).

Example :_test:SGEN:PDAT1:PULS:WIDTh 15e-9
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:WIDTh 10e-9
 :_test:SGEN:PPUL1:PULS:WIDTh 15e-9
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:WIDTh 10e-9
 :_test:MOD2:CONN3:PULS:WIDTh 20e-9

:PULSe:WIDTh?

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:WIDTh?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:WIDTh?
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:WIDTh?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:WIDTh?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:WIDTh?

Return Value Returns the current pulse width value.

Example :_test:SGEN:PDAT1:PULS:WIDTh?
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:WIDTh?
 :_test:SGEN:PPUL1:PULS:WIDTh?
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:WIDTh?
 :_test:MODULE2:CONNECTOR3:PULSE:WIDTh?
 might return:
 1.000000E-008

:PULSe:DCYClE

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:DCYClE <Duty Cycle>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:DCYClE
 <Duty Cycle>
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:DCYClE <Duty Cycle>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:DCYClE
 <Duty Cycle>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:DCYClE
 <Duty Cycle>

Parameters <Duty Cycle> Duty Cycle value in % (<NRf>).
 Sets the duty cycle of a repetitive pulse waveform.
 Valid range 0 ... 100.

Example :_test:SGEN:PDAT1:PULS:DCYC 25
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:DCYC 30
 :_test:SGEN:PPUL1:PULS:DCYC 25
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:DCYC 30
 :_test:mod2:conn3:pulse:DCYCLE 30

:PULSe:DCYClE?

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:DCYClE?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:DCYClE?
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:DCYClE?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:DCYClE?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:DCYClE?

Return Value Returns the current duty cycle value.

Example :_test:SGEN:PDAT1:PULS:DCYC?
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:DCYC?
 :_test:SGEN:PPUL1:PULS:DCYC?
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:DCYC?
 :_test:MOD2:CONNECTOR3:PULS:DCYCLE?

might return:

30

:PULSe:HOLD

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:HOLD <WIDTh | DCYClE>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:HOLD
 <WIDTh | DCYClE>
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:HOLD <WIDTh | DCYClE>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:HOLD
 <WIDTh | DCYClE>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:HOLD
 <WIDTh | DCYClE>

Parameters <WIDTh | DCYClE> The value to hold constant.

Specifies which parameter should remain constant when the period changes.

Example :_test:SGEN:PDAT1:PULS:HOLD DCYC
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:HOLD DCYC
 :_test:SGEN:PPUL1:PULS:HOLD DCYC
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:HOLD WIDT
 :_test:CGR:MOD2:CONN3:SOUR:PULS:HOLD WIDT

:PULSe:HOLD?

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:HOLD?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:HOLD?
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:HOLD?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:HOLD?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:HOLD?

Return Value Returns the parameter which is held constant when the period changes.

Example :_test:SGEN:PDAT1:PULS:HOLD?
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:HOLD?
 :_test:SGEN:PPUL1:PULS:HOLD?
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:HOLD?
 :_test:CGR:MOD2:CONN3:SOUR:PULS:HOLD?

might return:

DCYC

:PULSe:TRANSition[:LEADing]

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:TRANSition[:LEADing] <LeadingEdge>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:TRANSition[:LEADing] <LeadingEdge>
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:TRANSition[:LEADing] <LeadingEdge>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:TRANSition[:LEADing] <LeadingEdge>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:TRANSition[:LEADing] <LeadingEdge>

Parameters <LeadingEdge> Leading Edge value (<NRf>).

Sets the transition time for the LEADing edge. Only supported by E4838A frontends. The valid ranges are

E4838A: 0.5ns ... 5.0ns

Consider the following restrictions:

- When the specified port/terminal/connector is operating in NRZ format-mode, the actual value range is restricted by the selected period/frequency:
 - “:<Handle>:SGENeral:GLOBal:PERiod” on page 144
 - “:<Handle>:SGENeral:GLOBal:FREQuency” on page 145
 - “:MUX” on page 201
 - “:FORMat” on page 318
- When the specified port/terminal/connector is operating in RZ or R1 format-mode, the actual value range is restricted by the selected width or the duty cycle:
 - “:PULSe:WIDTh” on page 191
 - “:PULSe:DCYClE” on page 192
 - “:MUX” on page 201
 - “:FORMat” on page 318

Example :_test:SGEN:PDAT1:PULS:TRAN 2e-9
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:TRAN:LEAD
 :_test:SGEN:PPUL1:PULS:TRAN 2e-9
 :_test:SGEN:PPUL1:TERM1:SOUR:PULS:TRAN:LEAD 5e-9
 :_test:MOD2:CONN3:PULS:TRAN 5e-9

:PULSe:TRANsition[:LEADing]?

Syntax :<HANDLE>:SGENeral:PDATa(*)[:SOURce]:PULSeTRANsition[:LEADing]?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:TRANsition[:LEADing]?
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSeTRANsition[:LEADing]?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:TRANsition[:LEADing]?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:TRANsition[:LEADing]?

Return Value Returns the transition time for the leading edge.

Example :_test:SGEN:PDAT1:PULS:TRAN?
 :_test:SGEN:PDAT1:TERM1:SOUR:PULS:LEAD?
 :_test:SGEN:PDAT1:PULS:TRAN?
 :_test:SGEN:PPUL:TERM1:SOUR:PULS:LEAD?
 :_test:MOD2:CONN3:PULS:TRAN?

might return:

2.000000E-009

:PULSe:TRANsition:TRAILing

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:TRANsition:TRAILing<TrailingEdge>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:TRANsition:TRAILing<TrailingEdge>
 :<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:TRANsition:TRAILing<TrailingEdge>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:TRANsition:TRAILing<TrailingEdge>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:TRANsition:TRAILing<TrailingEdge>

Parameters <TrailingEdge> Trailing Edge value (<NRf>).

Sets the transition time for the trailing edge.

Only supported by E4838A frontends. The valid ranges are:

E4838A: 0.5ns ... 5.0ns

Consider the following restrictions:

- When the specified port/terminal/connector is operating in NRZ format-mode, the actual value range is restricted by the selected period/frequency:
 - “:<Handle>:SGENeral:GLOBal:PERiod” on page 144
 - “:<Handle>:SGENeral:GLOBal:FREQuency” on page 145
 - “:MUX” on page 201
 - “:FORMat” on page 318
- When the specified port/terminal/connector is operating in RZ or R1 format-mode, the actual value range is restricted by the selected width or the duty cycle:
 - “:PULSe:WIDTh” on page 191
 - “:PULSe:DCYClE” on page 192
 - “:MUX” on page 201
 - “:FORMat” on page 318

Example

```

:_test:SGEN:PDAT1:PULS:TRAN:TRA 2e-9
:_test:SGEN:PDAT1:TERM1:SOUR:PULS:TRAN:TRA 2e-9
:_test:SGEN:PPUL1:PULS:TRAN:TRA 2e-9
:_test:SGEN:PPUL1:TERM1:SOUR:PULS:TRAN:TRA 2e-9
:_test:CGR1:MOD2:CONN3:SOUR:PULS:TRAN:TRA 2e-9

```

:PULSe:TRANSition:TRAILing?

Syntax

```

:<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:TRANSition:TRAILing?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:TRANSition:TRAILing?
:<Handle>:SGENeral:PPULse(*):[:SOURce]:PULSe:TRANSition:TRAILing?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:PULSe:TRANSition:TRAILing?
:<Handle>[:CGRoup(*):MODule(*):CONNector(*):[:SOURce]:PULSe:TRANSition:TRAILing?

```

Return Value Returns the transition time for the TRAILing edge.

Example

```

:_test:SGEN:PDAT1:PULS:TRAN:TRA?
:_test:SGEN:PDAT1:TERM1:SOUR:PULS:TRAN:TRA?
:_test:SGEN:PPUL1:PULS:TRAN:TRA?

```

```
:_test:SGEN:PPUL1:TERM1:SOUR:PULS:TRAN:TRA?
```

```
:_test:CGR1:MOD2:CONN3:SOUR:PULS:TRAN:TRA?
```

might return:

```
2.000000E-009
```

:PULSe:TRANsition:CAConfiguration[:LEADing]

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:TRANsition:CAConfiguration[:LEADing] <ChannelAddLeadingEdge>

```
:<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:PULSe:TRANsition:CAConfiguration[:LEADing] <ChannelAddLeadingEdge>
```

```
:<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:TRANsition:CAConfiguration[:LEADing] <ChannelAddLeadingEdge>
```

```
:<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:TRANsition:CAConfiguration[:LEADing] <ChannelAddLeadingEdge>
```

```
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:TRANsition:CAConfiguration[:LEADing] <ChannelAddLeadingEdge>
```

Parameters <ChannelAddLeadingEdge> Additional Leading Edge value (<NRf>).

Sets the additional leading edge if the Channel Add mode is activated. This command is only supported for E4838A frontends in A2 channel-add mode (see “:OUTPut:CAConfiguration[:MODE]” on page 277).

The overall range is 0.5 ns to 5 ns. Consider the following restrictions:

- When the specified port/terminal/connector is operating in NRZ format-mode, the actual value range is restricted by the selected period/frequency:
 - “:<Handle>:SGENeral:GLOBal:PERiod” on page 144
 - “:<Handle>:SGENeral:GLOBal:FREQuency” on page 145
 - “:MUX” on page 201
 - “:FORMat” on page 318
- When the specified port/terminal/connector is operating in RZ or R1 format-mode, the actual value range is restricted by the selected width or the duty cycle:
 - “:PULSe:WIDTh” on page 191
 - “:PULSe:DCYClE” on page 192
 - “:MUX” on page 201

– “:FORMat” on page 318

NOTE “:PULSe:TRANsition:CAConfiguration:TRAILing” on page 199 holds actually the same value. Both parameters are cross-updated.

Example

```

:_test:SGEN:PDAT1:PULS:TRAN:CAC 2e-9
:_test:SGEN:PDAT1:TERM1:SOUR:PULS:TRAN:CAC:LEAD 3e-9
:_test:SGEN:PPUL1:PULS:TRAN:CAC 2e-9
:_test:SGEN:PPUL1:TERM1:SOUR:PULS:TRAN:CAC:LEAD 3e-9
:_test:MODULE2:CONNECTOR4:PULSE:TRANSITION:CACONFIGURATION 3e-9

```

:PULSe:TRANsition:CAConfiguration[:LEADing]?

Syntax

```

<Handle>:SGENeral:PDATa(*):[:SOURce]:PULSe:TRANsition
:CAConfiguration[:LEADing]?
<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:PULSe:TRANsition
:CAConfiguration[:LEADing]?
<Handle>:SGENeral:PPULse(*):[:SOURce]:PULSe:TRANsition
:CAConfiguration[:LEADing]?
<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:PULSe:TRANsition
:CAConfiguration[:LEADing]?
<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):[:SOURce]:PULSe
:TRANsition:CAConfiguration[:LEADing]?

```

Return Value Returns the additional transition-time of an E4838A frontend in A2 channel-add mode.

Example

```

:_test:SGEN:PDAT1:PULS:TRAN:CAC?
:_test:SGEN:PDAT1:TERM1:SOUR:PULS:TRAN:CAC:LEAD?
:_test:SGEN:PPUL1:PULS:TRAN:CAC?
:_test:SGEN:PPUL1:TERM1:SOUR:PULS:TRAN:CAC:LEAD?
:_test:MODULE2:CONNECTOR4:PULSE:TRANSITION:CACONFIGURATION?

```

might return:

```
2.000000E-009
```

:PULSe:TRANsition:CAConfiguration:TRAILing

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:PULSe:TRANsition:CAConfiguration:TRAILing <ChannelAddTrailingEdge>

:<Handle>:SGENeral:PPULse(*)[:SOURce]:PULSe:TRANsition:CAConfiguration:TRAILing <ChannelAddTrailingEdge>

:<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:PULSe:TRANsition:CAConfiguration:TRAILing <ChannelAddTrailingEdge>

:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:PULSe:TRANsition:CAConfiguration:TRAILing <ChannelAddTrailingEdge>

Parameters <ChannelAddTrailingEdge> Additional Trailing Edge value (<NRF>).

Description Sets the additional trailing edge, if the *Channel Add* mode is activated. This command is only supported for E4838A frontends in A2 channel-add mode (see “:OUTPut:CAConfiguration[:MODE]” on page 277).

The overall range is 0.5 ns to 5 ns. Consider the following restrictions:

- When the specified port/terminal/connector is operating in NRZ format-mode, the actual value range is restricted by the selected period/frequency:
 - “:<Handle>:SGENeral:GLOBal:PERiod” on page 144
 - “:<Handle>:SGENeral:GLOBal:FREQuency” on page 145
 - “:MUX” on page 201
 - “:FORMat” on page 318
- When the specified port/terminal/connector is operating in RZ or R1 format-mode, the actual value range is restricted by the selected width or the duty cycle:
 - “:PULSe:WIDTh” on page 191
 - “:PULSe:DCYClE” on page 192
 - “:MUX” on page 201
 - “:FORMat” on page 318

NOTE “:PULSe:TRANsition:CAConfiguration[:LEADing]” on page 197 holds actually the same value. Both parameters are cross-updated.

Example : _test:SGEN:PDAT1:PULS:TRAN:CAC:TRA 2e-9
 : _test:SGEN:PPUL1:PULS:TRAN:CAC:TRA 2e-9
 : _test:SGEN:PPUL1:TERM1:SOUR:PULS:TRAN:CAC:TRA 3e-9
 : _test:MOD2:CONN4:PULS:TRAN:CAC:TRA 4e-9

:PULSe:TRANsition:CAConfiguration:TRAILing?

Syntax :<Handle>:SGENeral:**PDATa**(*):[:SOURce]:PULSe:TRANsition:
 CAConfiguration:TRAILing?
 :<Handle>:SGENeral:**PDATa**(*):**TERMinal**(*):[:SOURce]:PULSe:TRANsition
 :CAConfiguration:TRAILing?
 :<Handle>:SGENeral:**PPULse**(*):[:SOURce]:PULSe:TRANsition:
 CAConfiguration:TRAILing?
 :<Handle>:SGENeral:**PPULse**(*):**TERMinal**(*):[:SOURce]:PULSe:TRANsition
 :CAConfiguration:TRAILing?
 :<Handle>[:CGRoup(*):MODule(*):**CONNector**(*):[:SOURce]:PULSe:
 TRANsition:CAConfiguration:TRAILing?

Return Value Returns the additional transition-time of an E4838A frontend in A2 channel-add mode.

Example : _test:SGEN:PDAT1:PULS:TRAN:CAC:TRA?
 : _test:SGEN:PDAT1:TERM1:SOUR:PULS:TRAN:CAC:TRA?
 : _test:SGEN:PPUL1:PULS:TRAN:CAC:TRA?
 : _test:SGEN:PPUL1:TERM1:SOUR:PULS:TRAN:CAC:TRA?
 : _test:MOD2:CONN4:PULS:TRAN:CAC:TRA?
 might return:
 2.000000E-009

:MUX

Syntax :<Handle>:SGENeral:PDATa(*):MUX <MUX Factor>
 :<Handle>:SGENeral:PPULse(*):MUX <MUX Factor>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):MUX <MuxFactor>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):MUX <NRf>

Parameters <NRf1> MUX factor = Multiply Factor for the individual port or connector.

In addition to the “system” MUX factor (segment resolution) it is possible to set the frequency multiply factor for individual ports, terminals or connectors to generate multiple or fraction of 2 data streams, like $f/2$ or $2f$ etc. The default value is 1. Valid values are $1/16 \dots 16$ at every factor of 2 (1/16, 1/8, etc.).

For the E4861A module, this range is expanded to $1/64 \dots 64$.

For the E4861B module, this range is expanded to $1/128 \dots 128$.

For the N4872A ... N4875A modules, this range is $1/512 \dots 512$.

The range of this parameter depends on the value of the system MUX factor (see “:<Handle>:SGENeral:GLOBal:MUX” on page 146).

Example :_test:SGEN:PDAT1:MUX 4
 :_test:SGEN:PPUL1:MUX 4
 :_test:SGEN:PPUL1:TERM1:MUX 0.5
 :_test:CGR1:MOD1:CONN1:MUX 2

:MUX?

Syntax :<Handle>:SGENeral:PDATa(*):MUX?
 :<Handle>:SGENeral:PPULse(*):MUX?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):MUX?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):MUX?

Return Value Returns the current frequency multiply factor (MUX factor) for the specified port, terminal or connector.

Example :_test:SGEN:PDAT1:MUX?
 :_test:SGEN:PPUL1:MUX?
 :_test:SGEN:PPUL1:TERM1:MUX?

:_test:CGR1:MOD1:CONN1:MUX?

might return:

6.25E-2

Parameter Commands for MUX and DEMUX Modules

Available Parameter Commands All new commands to set the properties of the MUX and DEMUX modules are found under:


:<Handle>[:CGROUP*]:MODULE*:CONNECTOR*

The following commands are available:


Parameter Group	Parameter	Command (on page)	Available on			
			E4868A	E4868B	E4869A	E4869B
Speed Parameters	Predefined Frequency		X	X	X	X
	Period	":<Handle>:SGENERal:GLOBal:PERiod" on page 144	X	X	X	X
	Frequency	":<Handle>:SGENERal:GLOBal:FREQuency" on page 145	X	X	X	X
Voltage Configuration	Amplitude	":VOLTage:AMPLitude" on page 206	X	X		
	Offset	":VOLTage:OFFSet" on page 207		X		
	Offset Enabling	":VOLTage:OFFSet:EN-ABLE" on page 208		X		
	External Attenuator	":OUTPut:EATTenuator" on page 209	X	X		
Delay Correction and Calibration	Delay Value	":OUTPut:DELay:SWEEP" on page 210	X	X		
	Delay Mode	":OUTPut:DELay:SWEEP:MODE" on page 211	X	X		
	Delay Storage Handling	":OUTPut:DELay:SWEEP:PRoM" on page 213	X	X		
Offset Compensation	":INPut:OCOMPensa-tion" on page 214			X		

Parameter Group	Parameter	Command (on page)	Available on			
			E4868A	E4868B	E4869A	E4869B
Threshold		":INPut:THReshold" on page 251			X	X
Sampling Phase Adjustment		":INPut:DELAy:SWEep" on page 259				X
Clock System	External Clock Input	":TRIGger" on page 215	X	X	X	X
	Clock Output (Subrate)	":TRIGger:MODE" on page 216	X	X		


Commands in the User Interface The following figure shows the output commands in the ParBERT user interface for a MUX module. Please note that not all commands are available for all modules. See the previous table for command availability.

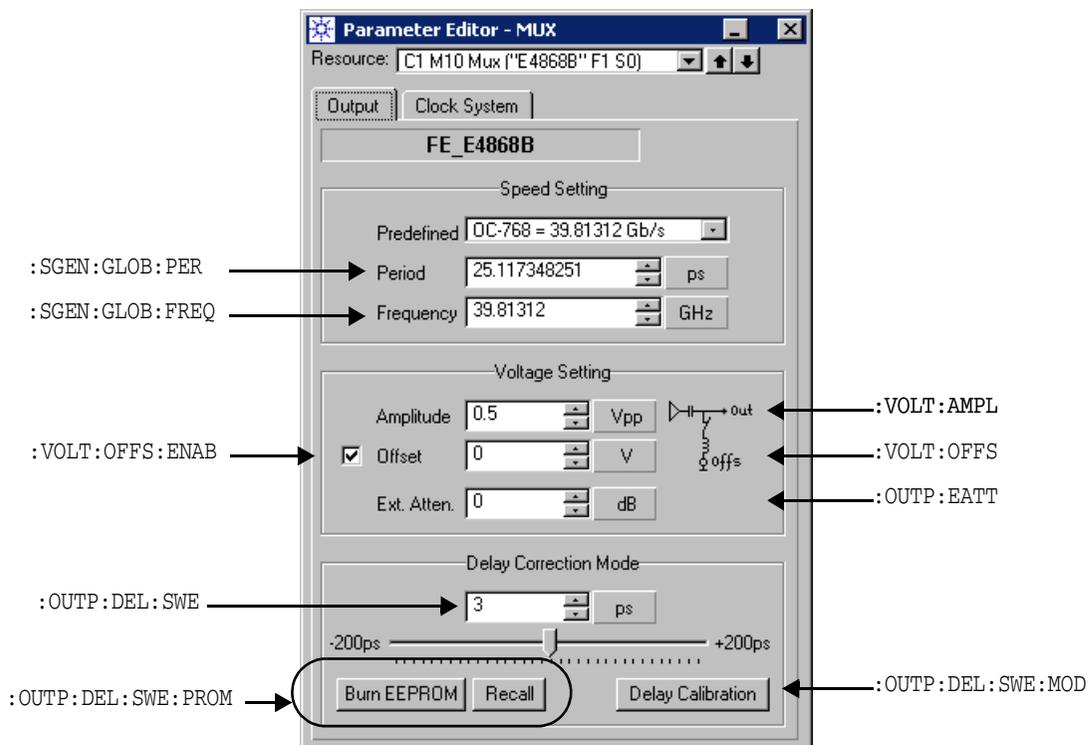


The following figures show the input commands in the ParBERT user interface for a DeMUX module. Please note that not all commands are available for all modules. See the previous table for command availability.

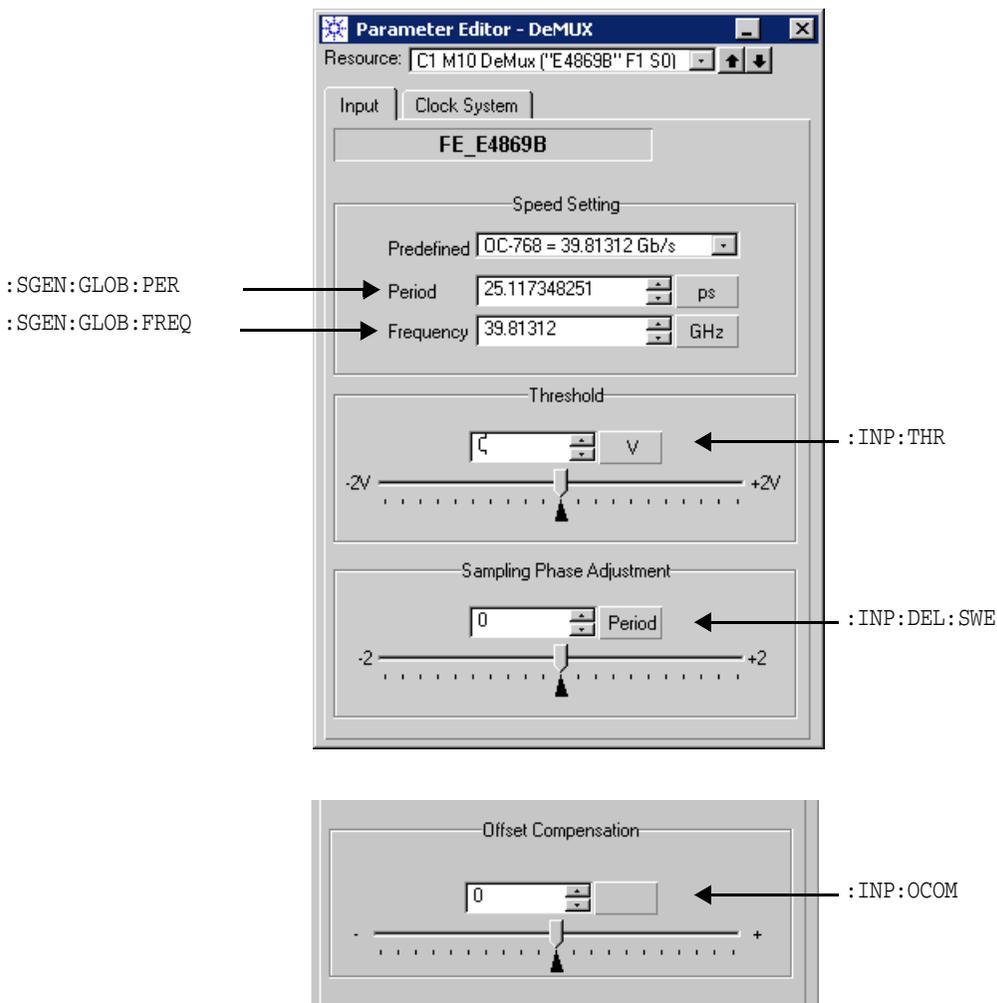

The following figure shows the clock system commands in the ParBERT user interface for a MUX module:

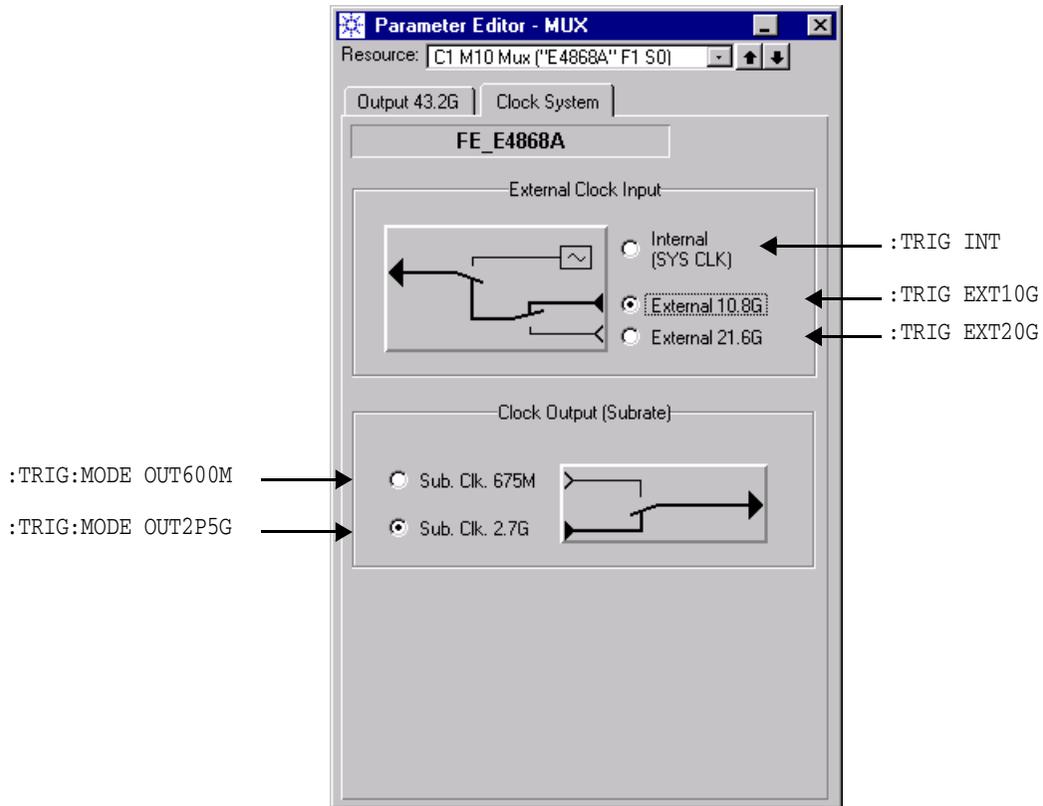

The following figure shows the clock system commands in the ParBERT user interface for a DeMUX module:

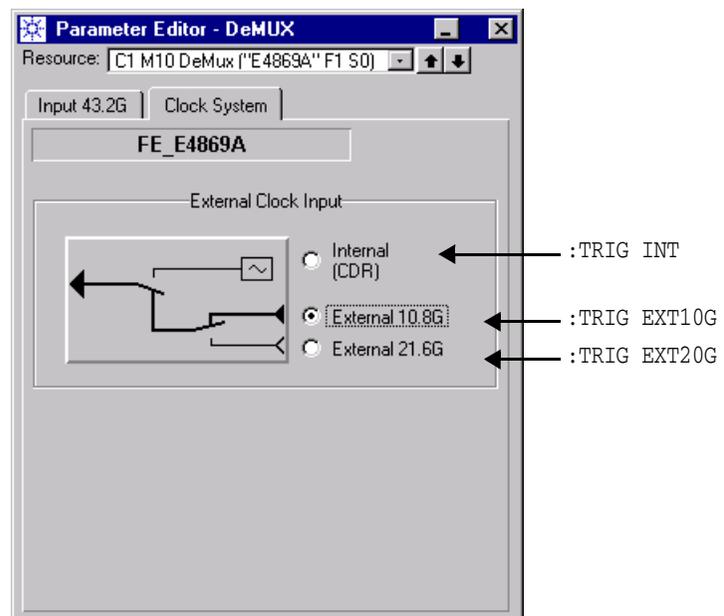

:VOLTage:AMPLitude

Syntax :<Handle>[:CGROUP*]:MODULE*:CONNECTOR* [:SOURCE]:VOLTage[:LEVEL:IMMEDIATE]:AMPLitude[:VALUE]<value>

Description Sets the amplitude of the output signal of the MUX module.

NOTE It is possible to set the amplitude to values higher than are given in the product overview without generating warnings. However, it cannot be guaranteed that the values are still within the specifications. This feature has been added to provide more useability (for example, for additional stressing of the DUT).

Related Commands

- “:VOLTage:OFFSet” on page 207
- “:OUTPut:EATTenuator” on page 209

NOTE Because the output of the E4868A MUX module is AC coupled, only the amplitude (peak-to-peak voltage) can be specified.

For the E4868B MUX module, an offset can be enabled or disabled.

Parameters <value> Voltage value in Volts. For valid values, see *Agilent ParBERT 81250 43G Parallel Bit Error Ratio Tester Product Overview*.

Example :_test:MOD10:CONN:VOLT:AMPL 1.0

:VOLTage:AMPLitude?

Syntax :<Handle>[:CGROUP*]:MODULE*:CONNECTOR* [:SOURCE]:VOLTage[:LEVEL:IMMEDIATE]:AMPLitude[:VALUE]?

Description Returns the amplitude of the output signal.

Return Value Voltage (in Volts).

Example :_test:MOD10:CONN:VOLT:AMPL?

might return:

1.0E+0

:VOLTage:OFFSet

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector* [:SOURce]:VOLTage[:LEVel:IMMEDIATE]:OFFSet[:VALue] <value>

NOTE This command is only available for the E4868B modules.

Parameters <value> Offset voltage to be added to the generated signal, see the hardware specifications for the range.

- Related Commands**
- “:VOLTage:AMPLitude” on page 206
 - “:VOLTage:OFFSet:ENABLE” on page 208
 - “:OUTPut:EATTenuator” on page 209

Example :_test:MOD10:CONN:VOLT:OFFS 0.5

:VOLTage:OFFSet?

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector* [:SOURce]:VOLTage[:LEVel:IMMEDIATE]:OFFSet[:VALue]?

Return Value Returns the offset voltage (offset added to the generated signal).

Example :_test:MOD10:CONN:VOLT:OFFS?

might return:

5.0E-1

:VOLTage:OFFSet:ENABle

Syntax :<Handle>[:CGROUP*]:MODULE*:CONNECTOR* [:SOURCE]:VOLTage[:LEVEL:IMMEDIATE]:OFFSet:ENABle <TRUE|FALSE>

NOTE This command is only available for the E4868B modules.

Description This command enables/disables voltage offset. If voltage offset is enabled and an external attenuator setting is specified, the offset voltage is checked and recalculated. If voltage offset is disabled, the offset voltage is ignored.

Related Commands

- “:VOLTage:AMPLitude” on page 206
- “:VOLTage:OFFSet” on page 207
- “:OUTPut:EATTenuator” on page 209

Parameters **TRUE** Enables voltage offset.

FALSE Disables voltage offset.

Example :_test:MOD10:CONN:VOLT:OFFS:ENAB TRUE

:VOLTage:OFFSet:ENABle?

Syntax :<Handle>[:CGROUP*]:MODULE*:CONNECTOR* [:SOURCE]:VOLTage[:LEVEL:IMMEDIATE]:OFFSet:ENABle?

Return Value Returns the current status of the voltage offset. See “:VOLTage:OFFSet:ENABle” on page 208 for a detailed description.

Example :_test:MOD10:CONN:VOLT:OFFS:ENAB?

might return:

TRUE

:OUTPut:EATTenuator

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*:OUTPut:EATTenuator <value>

Description This command allows you to enter the attenuation (in dB) of an external attenuator on the multiplexer's output. When this value is changed, the output values are also changed so that they reflect the values that actually reach the DUT (and not the values that reach the attenuator).

Related Commands

- “:VOLTage:AMPLitude” on page 206
- “:VOLTage:OFFSet” on page 207
- “:VOLTage:OFFSet:ENABle” on page 208

Parameters <value> Attenuation value of the external attenuator in dB; the range is dependent on the offset voltage.

Example :_test:_test:MOD10:CONN1:OUTP:EATT 20

:OUTPut:EATTenuator?

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*:OUTPut:EATTenuator?

Return Value Returns the attenuation value that was entered (manually or by the program) for the external attenuator in dB; range: 0 – 120 dB.

Example :_test:MOD10:CONN1:OUTP:EATT?
might return:
2.0E+1

:OUTPut:DELay:SWEep

- Syntax** :<Handle>[:CGRoup*]:MODule*:CONNector*:OUTPut:DELay:SWEep <sweep>
- Description** Manipulates globally the delay for all generators bound to the inputs of the E4868A module. The values set with this command are added to the start delay (see “:PULSe:DELay” on page 185) of those generators.

Parameters <sweep> The valid values depend on the current delay mode:

- Delay correction mode (TCOM): -200 ps to +200 ps.
- Delay calibration mode (DCAL): -2 ns to +2 ns

The current mode can be queried with “:OUTPut:DELay:SWEep:MODE?” on page 212.

Example In delay correction mode, set the delay to 3 ps:

```
:_test:MOD10:CONN1:OUTP:DEL:SWE 3E-12
```

In delay calibration mode, set the delay to -100 ps:

```
:_test:MOD10:CONN1:OUTP:DEL:SWE -100E-12
```

:OUTPut:DELay:SWEep?

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*:OUTPut:DELay:SWEep?

Description Returns the value for the delay.

Return Value The valid return values depend on the current delay mode:

- Delay correction mode: -200 ps to +200 ps.
- Delay calibration mode: -2ns to +2ns

The current mode can be queried with “:OUTPut:DELay:SWEep:MODE?” on page 212.

Example For delay correction mode:

```
:_test:MOD10:CONN1:OUTP:DEL:SWE?
```

might return:

```
3.0E-12
```

For delay calibration mode:

```
:_test:MOD10:CONN1:OUTP:DEL:SWE?
```

might return:

```
-1.0E-10
```

:OUTPut:DELay:SWEep:MODE

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*:OUTPut:DELay:SWEep:MODE
TCOM|DCAL

Description This command is used to switch between the delay correction and delay calibration mode.

If you receive one of the ParBERT 43G bundles, all frontends and MUX/DEMUX modules are factory-calibrated and ready to use. These two modes allows you to add a common delay to all the generator frontends connected to the MUX module.

The delay calibration sets the base value for the delay correction. If the delay calibration value is changed, the delay correction value is reset to zero.

The system stores two delay calibration values —one for an external clock source, one for the internal clock source. To set/query the currently selected clock source, see “:<Handle>:SGENeral:GLOBal:TRIGger[:SEQuence][:LAYer][:SOURce]” on page 173.

That means, the current delay value depends on the currently selected clock source and the current delay mode:

- If delay correction is set, the delay value depends on the delay calibration value (which depends on the selected clock source).
- If delay calibration (DCAL) is set, the delay value depends on the selected clock source.

Normally, the delay is automatically set with calibration tables, which enables the correct operation of the E4868A module.

Parameters <TCOM|DCAL> Mode to be set.

- **TCOM**
(Temperature **COM**ensation: Delay Correction) Switches into delay correction mode. This mode allows you to correct delay fluctuations caused by variations in ambient temperature well above 20 °C, for instance.
- **DCAL**
(Delay **CAL**ibration) Switches into delay calibration mode. This mode lets you recalibrate the delay if the clock module or the E4868A module was removed. This mode offers a wider timing range.

Example `:_test:MODule10:CONNector1:OUTPut:DELay:SWEEep:MODE TCOM`

or

`:_test:MODule10:CONNector1:OUTPut:DELay:SWEEep:MODE DCAL`

:OUTPut:DELay:SWEEep:MODE?

Syntax `<Handle>[:CGRoup*]:MODule*:CONNector*:OUTPut:DELay:SWEEep:MODE?`

Description This command returns the current delay mode.

Return Value **TCOM** (Temperature **COM**ensation: Delay Correction) The module is in delay correction mode. This mode allows you to correct delay fluctuations caused by variations in ambient temperature well above 20 °C, for instance.

DCAL (Delay **CAL**ibration) The module is in delay calibration mode. This mode lets you recalibrate the delay if the clock module or the E4868A module was removed. This mode offers a wider timing range.

Example `:_test:MODule10:CONNector1:OUTPut:DELay:SWEep:MODE?`
 might return:
 TCOM or DCAL

:OUTPut:DELay:SWEep:PROM

Syntax `:<Handle>[:CGRoup*]:MODule*:CONNector*.:OUTPut:DELay:SWEep:PROM
 STORe | RECall`

Description The delay values of an E4868 MUX module consist of three values: One delay calibration value if the built-in clock module generates the system clock, one delay calibration value if an external clock source is used, and one delay correction value. These values are stored in an EEPROM inside the module. They are hence non-volatile and independent of the ParBERT controller or the loaded setting.

If you change the delay values, your changes take immediate effect and remain effective until the ParBERT system is switched off. They are stored in the module. They remain effective, even if you terminate and restart the ParBERT user interface. But if you restart the ParBERT system, the values stored in the EEPROM become effective.

This command allows you to burn the currently active values to the EEPROM, or to restore the current values to the defaults from the EEPROM.

- Related Commands**
- “*:OUTPut:DELay:SWEep*” on page 210
 - “*:OUTPut:DELay:SWEep:MODE*” on page 211

Parameters

STORe Writes the currently used delay parameters to the EEPROM.

RECall Overwrites the currently used delay parameters with the last stored values from the EEPROM.

Example `:_test:MOD10:CONN1:OUTP:DEL:SWE:PROM REC`

:INPut:OCOMpensation

NOTE Valid only for E4869A/B (DEMUX) modules.

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*::INPut:OCOMpensation <value>

Definition By default, the decision threshold for sampling the incoming signal is set according to the mean value of the data signal. This is adequate for pure PRBS data. In cases where the received pattern has an unbalanced ratio of zeros to ones, this command allows you to fine-tune the threshold to an appropriate value.

An inadequate offset can be suspected, if:

- None of the analyzer terminals could synchronize.
- All analyzer terminals did synchronize, but exhibit an abnormally high BER.
- Some analyzer terminals did synchronize but show a BER close to the synchronization threshold, while others did not synchronize at all.

See also “*How to Change the Input Parameters of a DEMUX Module*” in the *System User Guide* for further details.

Parameters <value> New value of offset compensation; range: ± 1 (corresponds to roughly ± 100 mV).

Example :_test:MOD10:CONN1:INP:OCOM 0.9

:INPut:OCOMpensation?

NOTE Valid only for E4869A/B (DMUX) modules.

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*::INPut:OCOMpensation?

Definition Returns value used for the offset compensation.

Return Value Current value for offset compensation; range: ± 1 (corresponds to roughly ± 100 mV).

Example :_test:MOD10:CONN1:INP:OCOM?

might return:

9.0E-1

:TRIGger

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector* :TRIGger[:SEQuence:LAYer: SOURce] INT|EXT10G|EXT20G

Description Sets the source of the clock signal used for the timing of the E4868A MUX module.

Parameters <INT | EXT10G | EXT20G>

INT When this is selected, the module uses the clock signal provided by the central clock module.

NOTE The SYS CLK output from the central clock module must be connected to the SYS CLK input of the MUX module.

EXT10G The module uses an external signal in the range of 10.8 GHz provided by an external clock generator. The external clock must be connected to the Ext.Clk. input port.

EXT20G The module uses an external signal in the range of 21.6 GHz. provided by an external clock generator.

Example DRSA:MOD10:CONN:TRIG INT
DRSA:MOD10:CONN:TRIG EXT10G
DRSA:MOD10:CONN:TRIG EXT20G

:TRIGger?

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector* :TRIGger[:SEQuence:LAYer: SOURce]?

Return Value Returns the source of the clock signal used for the timing of the E4868A multiplexer.

Example DRSA:MOD10:CONN:TRIG?
might return:
INT or EXT10G or EXT20G

:TRIGger:MODE

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*:TRIGger:MODE
OUT600M|OUT2P5G

Parameters <OUT600M | OUT2P5G> Specifies the speed of the substrate clock output signal.

- OUT600M
Provides a signal of up to 675 MHz at the substrate clock output connector.
- OUT2P5G
Provides a signal of up to 2.7 GHz at the substrate clock output connector.

Example DRSA:MOD10:CONN:TRIG:MODE OUT600M
DRSA:MOD10:CONN:TRIG:MODE OUT2P5G

:TRIGger:MODE?

Syntax :<Handle>[:CGRoup*]:MODule*:CONNector*:TRIGger:MODE?

Return Value Returns the speed of the substrate clock output signal. Can be either:

- OUT600M
Provides a substrate clock output signal in the range of 675 MHz.
- OUT2P5G
Provides a substrate clock output signal in the range of 2.7 GHz.

Example DRSA:MOD10:CONN:TRIG:MODE?

might return:

OUT600M or OUT2P5G

DeMUX Rewiring Parameter Commands

The following commands are available:

Parameter Group	Parameter	Command (on page)
Activation	Rewire	<i>":<Handle>:SGENeral:GLOBal:SYNChronization:REWire" on page 219</i>
Configuration	Rewiring Mode	<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RMODE" on page 220</i>
Verification	Rewiring Check	<i>":<Handle>:SGENeral:GLOBal:SYNChronization:RCH" on page 221</i>
Multi-Stages DEMUX Settings	Number of Stages	<i>":<Handle>:SGENeral:PDATA:DMUX:STAGe" on page 222</i>
	Number of Outputs	<i>":<Handle>:SGENeral:PDATA:DMUX:STAGe:OUT" on page 223</i>

The following figure shows the parameter commands in the Agilent 81250 user interface.

:SGEN:PDAT:DMUX:STAG2

The screenshot shows the 'Analyzer Synchronization' dialog box. It is divided into three main sections:

- General Synchronization Parameters:** Includes radio buttons for 'Auto. Bit Sync.', 'Auto. Phase Align.', and 'Auto. Delay Align.'. It also features dropdown menus for 'Bit Error Rate Threshold' (set to 10^{-6}) and 'Phase Accuracy' (set to 20%).
- DeMUX Rewiring Parameters:** Includes a radio button for 'ON' (selected) and 'OFF'. Below this is the 'Rewiring Mode' section with radio buttons for 'Automatic', 'Terminal Roundtrip', and 'Trace Detection' (selected). A 'Verify Rewiring' checkbox is checked. The 'Worst Case Rewiring Cycles' is set to 5 (~00:00:40). The 'Required Terminals' is set to 4.
- DeMUX Architecture:** Includes a 'Stages' dropdown set to 2. Below it is a table with columns 'Stage #' and 'Outputs per DeMUX':

Stage #	Outputs per DeMUX
Stage1	2
Stage2	2

Arrows from the left side of the image point to the following command strings:

- :SGEN:GLOB:SYNC:REW ON (points to the 'ON' radio button)
- :SGEN:GLOB:SYNC:REW OFF (points to the 'OFF' radio button)
- :SGEN:GLOB:SYNC:RMOD AUTO (points to the 'Automatic' radio button)
- :SGEN:GLOB:SYNC:RMOD TRO (points to the 'Terminal Roundtrip' radio button)
- :SGEN:GLOB:SYNC:RMOD TDET (points to the 'Trace Detection' radio button)
- :SGEN:GLOB:SYNC:RCH ON (points to the 'Verify Rewiring' checkbox)
- :SGEN:GLOB:SYNC:RCH OFF (points to the 'Verify Rewiring' checkbox)

Arrows from the right side of the image point to the following command strings:

- :SGEN:PDAT:DMUX:STAG1:OUT 2 (points to the '2' in the Stage1 'Outputs per DeMUX' field)
- :SGEN:PDAT:DMUX:STAG2:OUT 2 (points to the '2' in the Stage2 'Outputs per DeMUX' field)

:<Handle>:SGENeral:GLOBal: SYNChronization:REWire

Syntax :<Handle>:SGENeral:GLOBal:SYNChronizat:REWire ON|OFF

Description Switches the DeMUX rewiring on and off.

If DeMUX rewiring is switched on, DeMUX rewiring takes place when the measurement is started. There is no reaction of the system until rewiring is completed or failed. Because DeMUX rewiring can take a lot of time, it is recommended to set all other system parameters first.

For more information on DeMUX rewiring, please refer to “*Automatic Rewiring of Demultiplexer Terminals*” in the *Agilent 81250 Parallel Bit Error Ratio Tester System User Guide*.

Parameters <ON|OFF> Switches DeMUX rewiring on or off.

Example :_test:SGEN:GLOB:SYNC:REW ON
or
:_test:SGEN:GLOB:SYNC:REW OFF

:<Handle>:SGENeral:GLOBal: SYNChronization:REWire?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronizat:REWire?

Return Value Returns the current state of DeMUX rewiring.

Example :_test:SGEN:GLOB:SYNC:REW?
might return:
ON or OFF

:<Handle>:SGENeral:GLOBal: SYNChronization:RMODE

Syntax :<Handle>:SGENeral:GLOBal:SYNChronizat:RMODE <AUTO|TRO|TDET>

Parameters <AUTO | TRO | TDET> Sets the modes for DeMUX rewiring.

- AUTO

The automatic mode tries first to rewire with the trace detection method and, if that fails, with the terminal roundtrip method.

- TRO

(**T**erminal **R**oundtrip) Rewire takes place with the terminal roundtrip.

- TDET

(**T**race **D**ETection) Rewire takes place with the trace detection method.

For more information on DeMUX rewiring modes, please refer to “*DEMUX Rewiring Modes*” in the *Agilent 81250 Parallel Bit Error Ratio Tester System User Guide*.

Example :_test:SGENeral:GLOBal:SYNChronization:RMODE AUTO

or

:_test:SGENeral:GLOBal:SYNChronization:RMODE TRO

or

:_test:SGENeral:GLOBal:SYNChronization:RMODE TDET

:<Handle>:SGENeral:GLOBal:SYNChronization:RMODe?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronizat:RMODe?

Return Value Returns the current mode for DeMUX rewiring. Can be:

- **AUTO**
The automatic mode tries first to rewire with the trace detection method and, if that fails, with the terminal roundtrip method.
- **TRO**
(**T**erminal **R**oundtrip) Rewire takes place with the terminal roundtrip.
- **TDET**
(**T**race **D**ETection) Rewire takes place with the trace detection method.

Example :_test:SGENeral:GLOBal:SYNcchronization:RMODe?

might return:

AUTO or TRO or TDET

:<Handle>:SGENeral:GLOBal:SYNChronization:RCH

Syntax :<Handle>:SGENeral:GLOBal:SYNChronizat:RCHeck ON|OFF

Parameters <ON|OFF> Switches the rewire verify mode on or off.

If verify rewiring is switched on, the system performs additional inspections and complains about possible errors.

If verify rewiring is switched off, the system tries to ignore noncritical problems to carry out a measurement.

Example :_test:SGEN:GLOB:SYNC:RCH ON

or

:_test:SGEN:GLOB:SYNC:RCH OFF

:<Handle>:SGENeral:GLOBal:SYNChronization:RCH?

Syntax :<Handle>:SGENeral:GLOBal:SYNChronizat:RCHeck?

Return Value Returns the current rewire verify mode (on or off).

If verify rewiring is switched on, the system performs additional inspections and complains about possible errors.

If verify rewiring is switched off, the system tries to ignore noncritical problems to carry out a measurement.

Example :_test:SGEN:GLOB:SYNC:RCH?

might return:

ON or OFF


:<Handle>:SGENeral:PDATA:DMUX:STAGe

Syntax :<Handle>:SGENeral:PDATA*:DMUX:STAGe*[:VALUE]

Description Specifies the number of stages of the DeMUX module. To set this value, you need to know the architecture of the demultiplexer.

Parameters *. Number of stages of the DeMUX module.

Example For a demultiplexer with the following architecture:

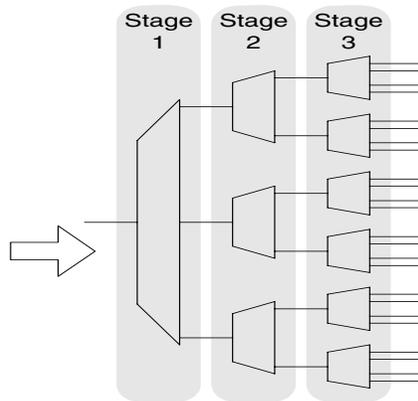

:_test:SGEN:PDATA:DMUX:STAG 3

:<Handle>:SGENeral:PDATA:DMUX:STAGe?

Syntax :<Handle>:SGENeral:PDATA*:DMUX:STAGe*[:VALUE]?

Description Returns the number of stages of the DeMUX module.

Return Value Number of stages.

Example :_test:SGEN:PDATA:DMUX:STAG?

might return:

3

:<Handle>:SGENeral:PDATA:DMUX:STAGe:OUT


Syntax :<Handle>:SGENeral:PDATA*:DMUX:STAGe*:OUTputs[:VALUE]<value>

Description Sets the number of outputs per DeMUX module for a specified stage.

Parameters * Index of the stage.

<value> Number of outputs per DeMUX module for a specified stage.

Example For a demultiplexer with the following architecture:

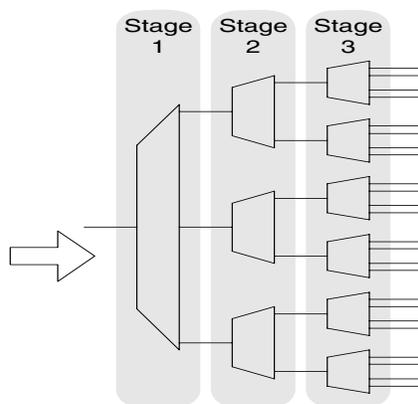

:_test:SGEN:PDATA:DMUX:STAG1:OUT 3

or

:_test:SGEN:PDATA:DMUX:STAG2:OUT 2

or

:_test:SGEN:PDATA:DMUX:STAG3:OUT 4

:<Handle>:SGENeral:PDATA:DMUX:STAGe: OUT?

Syntax :<Handle>:SGENeral:PDATA*:DMUX:STAGe*:OUTputs[:VALUE]?

Description Returns the number of outputs per DeMUX module for a specified stage.

Return Value Number of outputs per DeMUX module for a specified stage.

Example :_test:SGEN:PDATA:DMUX:STAG1:OUT?

might return:

3

Level Parameter Commands

The commands for specifying the level parameters are available on port, terminal and connector level. The parameters can be specified separately for pulse and data ports.

:VOLTage[:LEVel][:IMMediate]:HIGH

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH <HighLevel>

:<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH <HighLevel>

:<Handle>:SGENeral:PPULse(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH <HighLevel>

:<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH <HighLevel>

:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH <HighLevel>

Parameters <HighLevel> High Level value in Volts.

Sets the peak of a time varying signal.

Valid range depends on the frontend used:

E4838A: -2.15 to 4.40 V

E4843A: -1.75 to 3.10 V

These ranges are valid for a termination voltage of 0V (50 Ohm). With other termination voltages other values can be reached (for example, PECL Levels).

Example :_test:SGEN:PDAT1:VOLT:HIGH 3

:_test:SGEN:PDAT1:TERM1:SOUR:VOLT:LEV:IMM:HIGH 1

:_test:SGEN:PPUL1:VOLT:HIGH 3

:_test:SGEN:PPUL1:TERM1:SOUR:VOLT:LEV:IMM:HIGH 1.0

:_test:mod2:conn4:volt:high 2.5

:VOLTage[:LEVel][:IMMediate]:HIGH?

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH?
:<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH?
:<Handle>:SGENeral:PPULse(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH?
:<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH?
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:HIGH?

Return Value Returns the high voltage level of the signal.

Example :_test:SGEN:PDAT1:VOLT:HIGH?
:_test:SGEN:PDAT1:TERM1:SOUR:VOLT:LEV:IMM:HIGH?
:_test:SGEN:PPUL1:VOLT:HIGH?
:_test:SGEN:PPUL1:TERM1:SOUR:VOLT:LEV:IMM:HIGH?
:_test:MOD2:CONN4:VOLT:HIGH?

might return:

1.0000000E+000

:VOLTage[:LEVel][:IMMediate]:LOW

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW <LowLevel>

:<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW <LowLevel>

:<Handle>:SGENeral:PPULse(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW <LowLevel>

:<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW <LowLevel>

:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW <LowLevel>

Parameters <LowLevel> Low Level value in Volts (<NRF>).

Sets the low level of the time varying signal.

Valid range depends on the frontend used:

E4838A: -2.2 to 4.35 V

E4843A: -2.20 to 2.95 V

These ranges are valid for a termination voltage of 0V (50 Ohm). With other termination voltages other values can be reached (for example, PECL Levels).

Example :_test:SGEN:PDAT1:VOLT:LOW -1

:_test:SGEN:PDAT1:TERM1:SOUR:VOLT:LEV:IMM:LOW -1

:_test:SGEN:PPUL1:VOLT:LOW -1

:_test:SGEN:PPUL1:TERM1:SOUR:VOLT:LEV:IMM:LOW 0.1

:_test:MOD2:CONN4:VOLT:LOW 0.3

:VOLTage[:LEVel][:IMMediate]:LOW?

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW?
 :<Handle>:SGENeral:PPULse(*):[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW?
 :<Handle>[:CGRoup(*):MODULE(*):CONNector(*):[:SOURce]:VOLTage[:LEVel][:IMMediate]:LOW?

Return Value Returns the low voltage level.

Example :_test:SGEN:PDAT1:VOLT:LOW?
 :_test:SGEN:PDAT1:TERM1:SOUR:VOLT:LEV:IMM:LOW?
 :_test:SGEN:PPUL1:VOLT:LOW?
 :_test:SGEN:PPUL1:TERM1:SOUR:VOLT:LEV:IMM:LOW?
 :_test:MOD2:CONN4:VOLT:LOW?

might return:

-1.000000E+000

:VOLTage[:LEVel][:IMMEDIATE]: CAConfiguration:LOW

Syntax :<Handle>:SGENeral:PDATa(*)[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]
:CAConfiguration:LOW <AdditionalLowLevel>

:<Handle>:SGENeral:PDATa(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel]
[:IMMEDIATE]:CAConfiguration:LOW <AdditionalLowLevel>

:<Handle>:SGENeral:PPULse(*)[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]
:CAConfiguration:LOW <AdditionalLowLevel>

:<Handle>:SGENeral:PPULse(*):TERMinal(*)[:SOURce]:VOLTage[:LEVel]
[:IMMEDIATE]:CAConfiguration:LOW <AdditionalLowLevel>

:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:VOLTage[:LEVel]
[:IMMEDIATE]:CAConfiguration:LOW <AdditionalLowLevel>

Parameters <AdditionalLowLevel> Additional low level value in Volts (<NRf>).

Sets the additional low level of the pulse, which is available only when the A2 channel-add mode is selected for the port/terminal/connector (see “:OUTPut:CAConfiguration[:MODE]” on page 277).

This command is only supported for E4838A frontends.

For more details on the channel-add mode, see “How to Add Channels in Analog Mode” in the *Agilent 81250 System User Guide*.

Example :_test:SGEN:PDAT1:VOLT:CAC:LOW -2

:_test:SGEN1:PDAT1:TERM1:SOUR:VOLT:LEV:IMM:CAC:LOW 0.4

:_test:SGEN:PPUL1:VOLT:CAC:LOW -2

:_test:SGEN1:PPUL1:TERM1:SOUR:VOLT:LEV:IMM:CAC:LOW 0.4

:_test:CGR1:MOD2:CONN3:SOUR:VOLT:LEV:IMM:CAC:LOW 1

:VOLTage[:LEVel][:IMMEDIATE]: CAConfiguration:LOW?

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]
:CAConfiguration:LOW?

:<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:VOLTage[:LEVel]
[:IMMEDIATE]:CAConfiguration:LOW?

:<Handle>:SGENeral:PPULse(*):[:SOURce]:VOLTage[:LEVel][:IMMEDIATE]
:CAConfiguration:LOW?

:<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:VOLTage[:LEVel]
[:IMMEDIATE]:CAConfiguration:LOW?

:<Handle>[:CGRoup(*):]MODULE(*):CONNector(*):[:SOURce]:VOLTage[:LEVel]
[:IMMEDIATE]:CAConfiguration:LOW?

Return Value Returns the additional low-level of an E4838A frontend in A2 channel-add mode.

Example :_test:SGEN:PDAT1:VOLT:CAC:LOW?

:_test:SGEN1:PDAT1:TERM1:SOUR:VOLT:LEV:IMM:CAC:LOW?

:_test:SGEN:PPUL1:VOLT:CAC:LOW?

:_test:SGEN1:PPUL1:TERM1:SOUR:VOLT:LEV:IMM:CAC:LOW?

:_test:CGR1:MOD2:CONN3:SOUR:VOLT:LEV:IMM:CAC:LOW?

might return:

4.000000E-001

:VOLTage[:LEVel][:IMMEDIATE]:SEMode

Syntax :<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*)[:SOURCE]:VOLTage[:LEVel][:IMMEDIATE]:SEMode <New Value>

NOTE This command is only applicable to the N4868A 10.8G Booster modules. See the *System User Guide* for detailed information about how to work with the Booster modules.

Description Defines whether single-ended or differential channel operation mode should be used (TRUE = single-ended mode, FALSE = differential mode).

Parameter <New Value> New value used for the SEMode. When set to TRUE, single-ended mode is enabled. When set to FALSE, differential mode is enabled.

Example :_test:CGR1:MOD2:CONN3:SOUR:VOLT:LEV:IMM:SEM TRUE

:VOLTage[:LEVel][:IMMEDIATE]:SEMode?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:VOLTage[:LEVel] [:IMMEDIATE]:SEMode?

NOTE This command is only applicable to the N4868A 10.8G Booster modules. See the *System User Guide* for detailed information about how to work with the Booster modules.

Return Value Returns whether or not single-ended mode is currently enabled. When TRUE, single-ended mode is enabled. When FALSE, differential mode is enabled.

Example :_test:CGR1:MOD2:CONN3:SOUR:VOLT:LEV:IMM:SEM?

might return:

TRUE

:VOLTage[:LEVel][:IMMEDIATE]:SEMode:AVAILable?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*)[:SOURce]:VOLTage[:LEVel] [:IMMEDIATE]:SEMode:AVAILable?

NOTE This command is only applicable to the N4868A 10.8G Booster modules. See the *System User Guide* for detailed information about how to work with the Booster modules.

It is a good idea to implement this query in any SCPI scripts with the SEMode command to address future compatibility issues.

Return Value Returns whether or not single-ended mode is available.

Example :_test:CGR1:MOD2:CONN3:SOUR:VOLT:LEV:IMM:SEM:AVA?

might return:

TRUE

:SENSe:VOLTage:RANGe

Syntax :<Handle>:SGENeral:PDATa(*):SENSe:VOLTage:RANGe <range>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):SENSe:VOLTage:RANGe <range>
 :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):SENSe:VOLTage:RANGe
 <range>

Parameters <range> Selects the allowed input voltage range. For E4835A differential input frontends, two values are supported:

- 3 – allows input voltages –2 ... 3 V
- 5 – allows input voltages 0 ... 5 V

For E4863A, E4863B, E4865A, and E4867A frontends, the following values are supported:

- 0 – allows input voltages –2 ... 0 V
- 1 – allows input voltages –1 ... 1 V
- 2 – allows input voltages 0 ... 2 V

For N4873A and N4875A frontends, the selected value is the upper value of a 2 V range. For example, 1.5 defines a range of –0.5 ... 1.5 V.

Example :_test:SGEN:PDAT1:INP:RANG 3
 :_test:SGEN:PDAT1:TERM1:SENS:RANG 5
 :_test:CGROUP1:MODULE2:CONNECTOR4:SENSE:VOLTAGE:RANGE 3

:SENSe:VOLTage:RANGe?

Syntax :<Handle>:SGENeral:PDATa(*):SENSe:VOLTage:RANGe?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):SENSe:VOLTage:RANGe?
 :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):SENSe:VOLTage:RANGe?

Return Value Returns the currently selected input voltage range. See “:SENSe:VOLTage:RANGe” on page 233 for details.

Example :_test:SGEN:PDAT1:SENS:VOLT:RANG?
 :_test:SGEN:PDAT1:TERM1:SENS:VOLT:RANG?
 :_test:CGROUP1:MODULE2:CONNECTOR4:SENSE:VOLTAGE:RANGE?
 might return:
 3.0E+0

Amplitude/Offset Correction Factor Commands

These commands enable automatic correction for amplitude and offset errors caused by external attenuators, cable droop or equalizer circuits. They are supported by the following modules: E4861B, E4810A, E4811A, E4866A, E4867A, and N4872 ... N4875A.

The new parameters are:

- Offset Correction Factor (available for electrical generator and analyzer channels)
- Amplitude Correction Factor (available for electrical generator channels)
- Correction Factor Hold Mode (available for electrical generator channels)

These parameters are convenient functions for correcting for any changes in the signal voltage between the ParBERT and the DUT. The voltages of the signal leaving or arriving at the ParBERT are recalculated so that they correspond with the required signals of the DUT.

The value range for the correction factors is from 0.0 to 1.0, with 1.0 being the default value.

The values have to be understood as the multiplication factor that is required to calculate the levels at the DUT side, from the levels at the ParBERT side. A value of 0.0 has the special meaning of assuming AC-coupling. In this case, the generator levels will be symmetrical around 0 V with a termination voltage of 0 V. In the case of an analyzer channel, the termination voltage is forced to 0 V, while the threshold voltage remains untouched.

For correction factors other from 1.0, all the level parameters have to be considered being specified at the DUT side of the connection.

Note that the internal parameter checks have to deal with the levels at the frontends, so the error messages might show voltages that are different to what is specified for the DUT side.

If external attenuators have to be compensated, the offset and amplitude correction factor can be locked, so that changing one of both automatically sets the other one to the same value. In case of different values for offset and amplitude correction factor, the amplitude correction factor will be set to the offset correction value when locking is enabled.

:CALibration[:VOLTage]:OCFactor

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CALibration[:VOLTage]:OCFactor <ocfactor>
 :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK:CALibration[:VOLTage]:OCFactor <ocfactor>
 :<Handle>:SGENeral:PDATa(*):CALibration[:VOLTage]:OCFactor <ocfactor>
 :<Handle>:SGENeral:PDATa(*):CLOCK:CALibration[:VOLTage]:OCFactor <ocfactor>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration[:VOLTage]:OCFactor <ocfactor>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):CLOCK:CALibration[:VOLTage]:OCFactor <ocfactor>

Parameters <ocfactor> Offset correction factor; this can be in the range 0.0 ... 1.0. See “Amplitude/Offset Correction Factor Commands” on page 234 for details of this command.

Example :_test:SGEN:PDAT1:CAL:OCF 0.8

:CALibration[:VOLTage]:OCFactor?

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CALibration[:VOLTage]:OCFactor?
 :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK:CALibration[:VOLTage]:OCFactor?
 :<Handle>:SGENeral:PDATa(*):CALibration[:VOLTage]:OCFactor?
 :<Handle>:SGENeral:PDATa(*):CLOCK:CALibration[:VOLTage]:OCFactor?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration[:VOLTage]:OCFactor?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):CLOCK:CALibration[:VOLTage]:OCFactor?

Return Value Returns the current offset calibration factor. See “Amplitude/Offset Correction Factor Commands” on page 234 for details of this command.

Example `:_test:SGEN:PDAT1:CAL:OCF?`

might return:

8.0E-1

:CALibration[:VOLTage]:ACFactor

Syntax `<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CALibration[:VOLTage]:ACFactor <acfactor>`
`<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK:CALibration[:VOLTage]:ACFactor <acfactor>`
`<Handle>:SGENeral:PDATa(*):CALibration[:VOLTage]:ACFactor <acfactor>`
`<Handle>:SGENeral:PDATa(*):CLOCK:CALibration[:VOLTage]:ACFactor <acfactor>`
`<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration[:VOLTage]:ACFactor <acfactor>`
`<Handle>:SGENeral:PDATa(*):TERMinal(*):CLOCK:CALibration[:VOLTage]:ACFactor <acfactor>`

Parameters **<acfactor>** Amplitude correction factor; this can be in the range 0.0 ... 1.0. See “*Amplitude/Offset Correction Factor Commands*” on page 234 for details of this command.

Example `:_test:SGEN:PDAT1:CAL:ACF 0.75`

:CALibration[:VOLTage]:ACFactor?

Syntax `<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CALibration[:VOLTage]:ACFactor?`
`<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK:CALibration[:VOLTage]:ACFactor?`
`<Handle>:SGENeral:PDATa(*):CALibration[:VOLTage]:ACFactor?`
`<Handle>:SGENeral:PDATa(*):CLOCK:CALibration[:VOLTage]:ACFactor?`
`<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration[:VOLTage]:ACFactor?`
`<Handle>:SGENeral:PDATa(*):TERMinal(*):CLOCK:CALibration[:VOLTage]:ACFactor?`

Return Value Returns the current amplitude calibration factor. See “*Amplitude/Offset Correction Factor Commands*” on page 234 for details of this command.

Example `:_test:SGEN:PDAT1:CAL:ACF?`

might return:

7.5E-1

:CALibration[:VOLTage]:HOLD

Syntax `<Handle>:CGRoup(*):MODule(*):CONNector(*):CALibration[:VOLTage]:HOLD
<IND| LOCK>`

`<Handle>:CGRoup(*):MODule(*):CONNector(*):CLOCK:CALibration[:
VOLTage]:HOLD <IND| LOCK>`

`<Handle>:SGENeral:PDATa(*):CALibration[:VOLTage]:HOLD <IND| LOCK>`

`<Handle>:SGENeral:PDATa(*):CLOCK:CALibration[:VOLTage]:HOLD <IND|
LOCK>`

`<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration[:VOLTage]:HOLD
<IND| LOCK>`

`<Handle>:SGENeral:PDATa(*):TERMinal(*):CLOCK:CALibration[:VOLTage]:
HOLD <IND| LOCK>`

Parameters **<IND|LOCK>** Defines whether the offset and amplitude correction factors are independent (IND) or locked (LOCK). See *“Amplitude/Offset Correction Factor Commands” on page 234* for details of this command.

Example `:_test:sgen:pdatt1:cal:hold LOCK`

:CALibration[:VOLTage]:HOLD?

Syntax `<Handle>:CGRoup(*):MODule(*):CONNector(*):CALibration[:VOLTage]:
HOLD?`

`<Handle>:CGRoup(*):MODule(*):CONNector(*):CLOCK:CALibration[:
VOLTage]:HOLD?`

`<Handle>:SGENeral:PDATa(*):CALibration[:VOLTage]:HOLD?`

`<Handle>:SGENeral:PDATa(*):CLOCK:CALibration[:VOLTage]:HOLD?`

`<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration[:VOLTage]:HOLD?`

`<Handle>:SGENeral:PDATa(*):TERMinal(*):CLOCK:CALibration[:VOLTage]:
HOLD?`

Return Value Returns the current correction factor locking mode. See *“Amplitude/Offset Correction Factor Commands” on page 234* for details of this command.

Example `:_test:sgen:pdat1:cal:hold?`
 might return:
 LOCK

Delay Control Parameter Commands

The delay control parameter commands are available on port, terminal and connector level. The parameters can be specified separately for pulse and data ports.

:DCONtrol[:DEViation]?

Syntax

```
:<Handle>:SGENeral:PDATa(*):[:SOURce]:DCONtrol:[DEViation]?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:DCONtrol:[DEViation]?
:<Handle>:SGENeral:PPULse(*):[:SOURce]:DCONtrol:[DEViation]?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:DCONtrol:
[DEViation]?
:<Handle>[:CGRoup(*):MODULE(*):CONNector(*):[:SOURce]:DCONtrol:
[DEViation]?
```

Return Value Returns the current maximum delay control deviation in seconds.

Example

```
:_test:SGEN:PDAT1:DCONT?
:_test:SGEN:PDAT1:TERM1:SOUR:DCONT:DEV?
:_test:SGEN:PPUL1:DCONT?
:_test:SGEN:PPUL1:TERM1:SOUR:DCONT?
:_test:MODULE2:CONNECTOR3:DCONT:DEV?
```

might return:

```
5.0E-11
```

:DControl:SENSitivity

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:DControl:SENSitivity <Sensitivity>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:DControl:SENSitivity <Sensitivity>
 :<Handle>:SGENeral:PPULse(*):[:SOURce]:DControl:SENSitivity <Sensitivity>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:DControl:SENSitivity <Sensitivity>
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):[:SOURce]:DControl:SENSitivity <Sensitivity>

Description Sets the delay control sensitivity of the external delay control modulation signal.

Parameters <Sensitivity> Delay control sensitivity in seconds per volt (<NRf>).

Example :_test:SGEN:PDAT1:DCont:SENS 5.0E-10
 :_test:SGEN:PDAT1:TERM1:SOUR:DCont:SENS 5.0E-10
 :_test:SGEN:PPUL1:DCont:SENS 5.0E-11
 :_test:SGEN:PPUL1:TERM1:SOUR:DCont:SENS 5.0E-10
 :_test:MODULE2:CONNECTOR3:DControl:SENSITIVITY 5.0E-11

:DControl:SENSitivity?

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:DControl:SENSitivity?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:DControl:SENSitivity?
 :<Handle>:SGENeral:PPULse(*):[:SOURce]:DControl:SENSitivity?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:DControl:SENSitivity?
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):[:SOURce]:DControl:SENSitivity?

Return Value Returns the current delay control sensitivity in seconds per volt.

Example :_test:SGEN:PDAT1:DCont:SENS?
 :_test:SGEN:PDAT1:TERM1:SOUR:DCont:SENS?
 :_test:SGEN:PPUL1:DCont:SENS?
 :_test:SGEN:PPUL1:TERM1:SOUR:DCont:SENS?
 :_test:MODULE2:CONNECTOR3:DCONTROL:SENSITIVITY?
might return:
 5.0E-11

:DControl:SOURce

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:DControl:SOURce <NAV | EXT>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:DControl:SOURce
 <NAV | EXT>
 :<Handle>:SGENeral:PPULse(*):[:SOURce]:DControl:SOURce <NAV | EXT>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:DControl:SOURce
 <NAV | EXT>
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):[:SOURce]:DControl:SOURce
 <NAV | EXT>

Parameters <NAV | EXT> Sets the delay control source to either NAV (not available) or EXT (external).

The E4862B frontends support only EXT. All other frontends support only NAV.

Example :_test:SGEN:PDAT1:DCont:SOUR EXT
 :_test:SGEN:PDAT1:TERM1:SOUR:DCont:SOUR EXT
 :_test:SGEN:PPUL1:DCont:SOUR EXT
 :_test:SGEN:PPUL1:TERM1:SOUR:DCont:SOUR EXT
 :_test:MODULE2:CONNECTOR3:DCONTROL:SOURCE EXT

:DControl:SOURce?

Syntax :<Handle>:SGENeral:PDATA(*):[:SOURce]:DControl:SOURce?
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):[:SOURce]:DControl:SOURce?
 :<Handle>:SGENeral:PPULse(*):[:SOURce]:DControl:SOURce?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:DControl:SOURce?
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):[:SOURce]:DControl:
 SOURce?

Return Value Returns the current delay control source: either NAV (not available) or EXT (external).

The E4862B frontends support only EXT. All other frontends support only NAV.

Example :_test:SGEN:PDATA1:DCONT:SOUR?
 :_test:SGEN:PDATA1:TERM1:SOUR:DCONT:SOUR?
 :_test:SGEN:PPUL1:DCONT:SOUR?
 :_test:SGEN:PPUL1:TERM1:SOUR:DCONT:SOUR?
 :_test:MODULE2:CONNECTOR3:DCONTROL:SOURCE?

might return:

EXT

:DControl:State

NOTE Executing this command while the system is running causes the system to be restarted.

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:DControl:State <ON | OFF>
:<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:DControl:State <ON | OFF>
:<Handle>:SGENeral:PPULse(*):[:SOURce]:DControl:State <ON | OFF>
:<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:DControl:State <ON | OFF>
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):[:SOURce]:DControl:State <ON | OFF>

Parameters <ON | OFF> Switches the specified external delay control input connector on or off.

Example :_test:SGEN:PDAT1:DControl:State ON
:_test:SGEN:PPUL1:TERM1:SOUR:DControl:State ON
:_test:MODULE2:CONNECTOR3:DControl:State ON

:DControl:StAtE?

Syntax :<Handle>:SGENeral:PDATa(*):[:SOURce]:DControl:StAtE?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):[:SOURce]:DControl:StAtE?
:<Handle>:SGENeral:PPULse(*):[:SOURce]:DControl:StAtE?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):[:SOURce]:DControl:StAtE?
:<Handle>[:CGRoup(*):MODULE(*):CONNECTor(*):[:SOURce]:DControl:StAtE?

Return Value Returns the current state of the specified external delay control input connector.

Example :_test:SGEN:PDAT1:DControl:StAtE?
:_test:SGEN:PDAT1:TERM1:SOUR:DControl:StAtE?
:_test:SGEN:PPUL1:DControl:StAtE?
:_test:SGEN:PPUL1:TERM1:SOUR:DControl:StAtE?
:_test:MODULE2:CONNECTOR3:DControl:StAtE?

might return:

OFF

Input Parameter Commands

The input parameter commands are available on port, terminal and connector level.

:INPut[:STATe]

Syntax :<Handle>:SGENeral:PDATa(*)**:INPut[:STATe]** <ON | OFF>
 :<Handle>:SGENeral:PDATa(*)**:TERMinal(*)**:INPut[:STATe]**** <ON | OFF>
 :<Handle>[:CGRoup(*)]:MODule(*)**:CONNector(*)**:INPut[:STATe]**** <ON | OFF>

Parameters <ON | OFF> Switch the specified analyzer input connector ON or OFF.

Example :_test:SGEN:PDAT1:INPUT ON
 :_test:SGEN1:PDAT1:TERM1:INPUT ON
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPUT ON

:INPut[:STATe]?

Syntax :<Handle>:SGENeral:PDATa(*)**:INPut[:STATe]?** <NFORce | FORCe>
 :<Handle>:SGENeral:PDATa(*)**:TERMinal(*)**:INPut[:STATe]?****
 <NFORce | FORCe>
 :<Handle>[:CGRoup(*)]:MODule(*)**:CONNector(*)**:INPut[:STATe]?****
 <NFORce | FORCe>

Description Returns the current status of the specified analyzer input connector.

Parameters <NFORce | FORCe> Defines how the query is executed:

- NFORce
 Default value. Only the firmware is queried for the current state.
- FORCe
 When FORCe is entered, the firmware checks the current condition in the hardware. This is required to make sure that the input is really switched on, or to check if the protection circuit within the input has turned off the channel to protect it from damage.

NOTE The FORCe call is slower than NFORce.

Example : _test:SGEN:PDAT1:INPUT?
 : _test:SGEN1:PDAT1:TERM1:INPUT?
 : _test:CGROUP1:MODULE2:CONNECTOR4:INPUT?
might return:
 ON

:INPut:POLarity

Syntax :<Handle>:SGENeral:PDATa(*):INPut:POLarity <NORMal | INVerted>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:POLarity <NORMal | INVerted>
 :<Handle>:CGROUP(*):MODUle(*):CONNector(*):INPut:POLarity <NORMal | INVerted>

Parameters <NORMal | INVerted> Sets the input polarity of the specified *data* port/terminal/connector to either normal or inverted.

This command is not available for the E4863A/E4865A frontends and E4867A module.

Example : _test:SGEN:PDAT1:INP:POL INV
 : _test:SGEN:PDAT1:TERM1:INP:POL INV
 : _test:CGROUP1:MODULE2:CONNECTOR4:INPut:POLARITY NORM

:INPut:POLarity?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:POLarity?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:POLarity?
 :<Handle>:CGROUP(*):MODUle(*):CONNector(*):INPut:POLarity?

Return Value Returns the input polarity of the specified port/terminal/connector. The return value is either NORMal or INVerted.


Example : _test:SGEN:PDAT1:INP:POL?
 : _test:SGEN:PDAT1:TERM1:INP:POL?
 : _test:CGROUP1:MODULE2:CONNECTOR4:INPut:POLARITY?
might return:
 NORM

:INPut:TYPE

Syntax :<Handle>:SGENeral:PDATa(*):INPut:TYPE <BALanced | NORMal | INVerted>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:TYPE <BALanced | NORMal | INVerted>
 :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):INPut:TYPE <BALanced | NORMal | INVerted>

Parameters <BALanced | NORMal | INVerted> Selects how the differential input frontends are sampled.

- BALanced selects differential operation (this is the reset value).
- NORMal compares the normal input against a threshold value.
- INVerted compares the complement input against a threshold value.

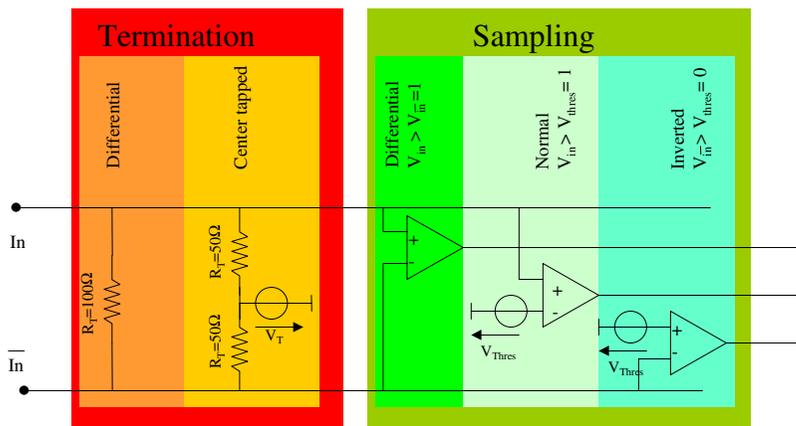

In NORMal and INVerted operation (“:INPut:IMPedance[:INTernal]” on page 252 and “:INPut:TVOLTage” on page 250) specify the termination of the input.

In BALanced operation the termination is not used, but is checked against absolute limits. “:INPut:SERial” on page 254 is also ignored in BALanced operation, but is checked against absolute limits.

Example :_test:SGEN:PDAT1:INP:TYPE BAL
 :_test:SGEN:PDAT1:TERM1:INP:TYPE INV
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:TYPE NORM

:INPut:TYPE?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:TYPE?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:TYPE?
 :<Handle>:CGRoup(*):MODule(*):CONNector(*):INPut:TYPE?

Return Value Returns the operation mode of the differential input frontend.

Example :_test:SGEN:PDAT1:INP:TYPE?
 :_test:SGEN:PDAT1:TERM1:INP:TYPE?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:TYPE?
 might return:


BAL

:INPut:MODE

Syntax :<Handle>:SGENeral:PDATa(*):INPut:MODE <DIFF | SNOR | SCOM>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:MODE <DIFF | SNOR | SCOM>
 :<Handle>:CGRoup(*):MODule(*):CONNector(*):INPut:MODE <DIFF | SNOR | SCOM>


Parameters <DIFF | SNOR | SCOM> Selects between single-ended operation and differential operation modes (if supported by the frontend).

- DIFF selects differential frontend operation. Termination is done according to :INPut:TCONfig, comparator operation is selected according to :INPut:MODE (this is the reset value).
- SNOR configures the frontend to single-ended operation using the normal input as shown in the following picture:

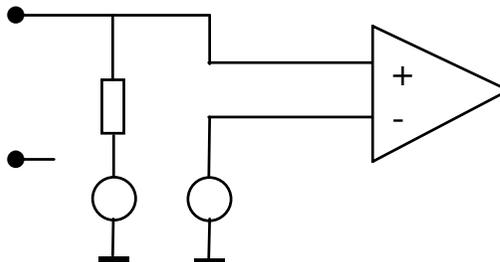

Note that :INPut:TCONfig and :INPut:MODE is ignored in this case.

- SCOM configures the frontend to single-ended operation using the complement input according to the following picture:

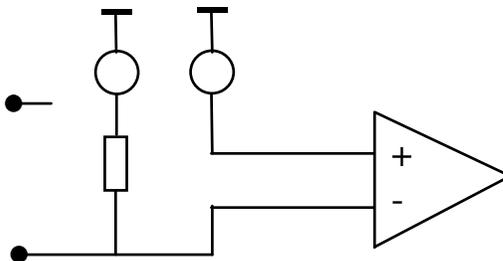

Note that :INPut:TCONfig and :INPut:MODE is ignored in this case.

Example :_test:SGEN:PDAT1:INP:MODE DIFF
 :_test:SGEN:PDAT1:TERM1:INP:MODE SNOR
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:MODE SCOM

:INPut:MODE?

Syntax :<Handle>:SGENeral:PDATa(*) :INPut:MODE?
 :<Handle>:SGENeral:PDATa(*) :TERMinal(*) :INPut:MODE?
 :<Handle>:CGROUP(*) :MODule(*) :CONNector(*) :INPut:MODE?

Return Value Returns the operation mode of an input frontend.

Example :_test:SGEN:PDAT1:INP:MODE?
 :_test:SGEN:PDAT1:TERM1:INP:MODE?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:MODE?

might return:

SNOR

:INPut:TVOLtage

Syntax :<Handle>:SGENeral:PDATa(*):INPut:TVOLtage <TerminationVoltage>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:TVOLtage
 <TerminationVoltage>
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNector(*):INPut:TVOLtage
 <TerminationVoltage>

Parameters <TerminationVoltage> Termination voltage (<NRf>).

Specifies the termination voltage of an analyzer input connector. The termination voltage range of the available analyzer frontends is -2.1 V to +3.1 V.

Example :_test:SGEN:PDAT1:INP:TVOL -2
 :_test:SGEN1:PDAT1:TERM1:INP:TVOL -2
 :_test:CGROUP1:MODULE2:CONNECTOR4:INP:TVOL -2

:INPut:TVOLtage?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:TVOLtage?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:TVOLtage?
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNector(*):INPut:TVOLtage?

Return Value Returns the current termination voltage of the specified analyzer input connector.

Example :_test:SGEN:PDAT1:INP:TVOL?
 :_test:SGEN1:PDAT1:TERM1:INP:TVOL?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INP:TVOL?
 might return:
 -2.000000E+000

:INPut:THReshold

Syntax :<Handle>:SGENeral:PDATa(*):INPut:THReshold <Threshold>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:THReshold <Threshold>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:THReshold
 <Threshold>

Parameters <Threshold> Threshold value in volts (<NRf>). Specifies the threshold voltage of an analyzer input connector.

Example :_test:SGEN:PDAT1:INPut:THR 1
 :_test:SGEN1:PDAT1:TERM1:INPut:THR 1
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:THR 1

:INPut:THReshold?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:THReshold?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:THReshold?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:THReshold?

Return Value Returns the current threshold voltage of the specified analyzer input connector.

Example :_test:SGEN:PDAT1:INPut:THR?
 :_test:SGEN1:PDAT1:TERM1:INPut:THR?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:THR?
 might return.
 1.000000E+000

:INPut:IMPedance[:INTernal]

Syntax :<Handle>:SGENeral:PDATa(*):INPut:IMPedance[:INTernal] <Impedance>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:IMPedance[:INTernal]
 <Impedance>
 :<Handle>[:CGRoup(*):MODUle(*):CONNeCtor(*):INPut:IMPedance[:
 INTernal] <Impedance>

Parameters <Impedance> Internal termination impedance value.

Specifies the internal termination impedance of the analyzer input connector. To set 10 kOhm impedance, use -1 in the command. For 50 Ohm impedance, use 50 in the command.

Example :_test:SGEN:PDAT1:INPut:IMP -1
 :_test:SGEN1:PDAT1:TERM1:INPut:IMP -1
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:IMP -1

:INPut:IMPedance[:INTernal]?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:IMPedance[:INTernal]?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:IMPedance[:INTernal]?
 :<Handle>[:CGRoup(*):MODUle(*):CONNeCtor(*):INPut:IMPedance[:
 INTernal]?

Return Value Returns the current internal impedance of the specified analyzer input connector. A negative value relates to the HiZ internal impedance.

Example :_test:SGEN:PDAT1:INPut:IMP?
 :_test:SGEN1:PDAT1:TERM1:INPut:IMP?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:IMP?
 might return:
 -1.000000E+000

:INPut:SEQuence:[LAYer:SOURce:]CLOCK

Syntax :<Handle>:SGeneral:PData:INPut:SEQuence:[LAYer:SOURce:]CLOCK
 <INTernal | CDR>
 :<Handle>:SGeneral:PData:TERMinal:INPut:SEQuence:[LAYer:SOURce:]
]CLOCK <INTernal | CDR>

```
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:SEQuence:[LAYer:
SOURce:]CLOCK <INTernal | CDR>
```

Description Sets the clock source for a module to either normal or CDR feedback mode. In normal mode, the module relies on the GCLK provided by the central. In CDR feedback mode, the CDR output of the module is fed back to itself. This command can only be used when the system is stopped.

The CDR feedback mode can only be activated for an N4873A/75A data module.

Parameters <INTernal | CDR> Sets the clock source for a module to either normal or CDR feedback mode.

Examples

```
:_test:SG:PD:INP:SEQ:CLOC CDR
:_test:SG:PD:TERM:INP:SEQ:CLOC CDR
:_test:CGR1:MOD1:CONN:INP:SEQ:CLOC CDR
```

:INPut:SEQuence:[LAYer:SOURce:]CLOCK?

Syntax

```
:<Handle>:SGeneral:PData:INPut:SEQuence:[LAYer:SOURce:]CLOCK?
:<Handle>:SGeneral:PData:TERMinal:INPut:SEQuence:[LAYer:SOURce:]
CLOCK?
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:SEQuence:[LAYer:
SOURce:]CLOCK?
```

Return Value Returns the currently used clock source mode for a module. This can be either INTernal (normal mode) or CDR (CDR feedback mode).

Example

```
:_test:cgr1:mod1:conn1:inp:seq:cloc?
might return:
INT
```

:INPut:SERIal

Syntax :<Handle>:SGENeral:PDATa(*):INPut:SERIal <Impedance>
 :<Handle>:SGENeral:PDATa(*):TERMIal(*):INPut:SERIal <Impedance>
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNEctor(*):INPut:SERIal <Impedance>

Parameters <Impedance> Serial impedance value.

Specifies a serial impedance on the specified analyzer input connector. The reset value is 0.

For electronic devices that are not able to drive a 50-Ohm input, an additional serial resistor is used. The specified value is taken into account to calculate the corresponding threshold.

Example :_test:SGEN:PDAT1:INPut:SER 50
 :_test:SGEN1:PDAT1:TERM1:INPut:SER 50
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:SER 50

:INPut:SERIal?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:SERIal?
 :<Handle>:SGENeral:PDATa(*):TERMIal(*):INPut:SERIal?
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNEctor(*):INPut:SERIal?

Return Value Returns the current serial impedance used for the specified analyzer input connector.

Example :_test:SGEN:PDAT1:INPut:SER?
 :_test:SGEN1:PDAT1:TERM1:INPut:SER?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:SER?
 might return:
 5.000000E+001

:INPut:DELay

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELay <Delay>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELay <Delay>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:DELay <Delay>

Parameters <Delay> Specifies the delay of the sampling edge (<NRF>). It can be specified in seconds or in cycles (take into account the MUX-factor or in other words the “oversampling factor”).

If this command is used, the value will be interpreted as a timing value only. Therefore, :INPut:DELay:CYCLes is set to zero.

Otherwise, if the delay is specified by :INPut:DELay:CYCLes and :INPut:DELay:TIME, the corresponding delay will be calculated. The number of cycles is converted into seconds and added to the specified :INPut:DELay:TIME value.

Example :_test:SGEN:PDAT1:INPut:DEL 50e-9
 :_test:SGEN1:PDAT1:TERM1:INPut:DEL 50e-9
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DEL 50e-9

:INPut:DELay?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELay?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELay?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:DELay?

Return Value Returns the current delay of the sampling edge for the specified analyzer input connector.

Example :_test:SGEN:PDAT1:INPut:DEL?
 :_test:SGEN1:PDAT1:TERM1:INPut:DEL?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DEL?

might return:

5.000000E-008

:INPut:DELAy:CYCLes

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELAy:CYCLes <Cycles>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELAy:CYCLes <Cycles>
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNector(*):INPut:DELAy:CYCLes
 <Cycles>

Parameters <Cycles> 1 cycle corresponds to the actual period/frequency valid for the specified analyzer input connector.

If the delay is specified by DELAy:CYCLes and :INPut:DELAy:TIME, the corresponding delay will be calculated. The number of cycles is converted into seconds and added to the specified :INPut:DELAy:TIME value.

If :INPut:DELAy is used, the value will be interpreted as a timing value only. Therefore, :INPut:DELAy:CYCLes is set to zero.

Example :_test:SGEN:PDAT1:INPut:DELAy:CYCL 0.5
 :_test:SGEN1:PDAT1:TERM1:INPut:DELAy:CYCL 0.5
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DELAy:CYCL 0.5

:INPut:DELAy:CYCLes?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELAy:CYCLes?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELAy:CYCLes?
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNector(*):INPut:DELAy:CYCLes?

Return Value Returns the current cycle value of the sampling edge for the specified analyzer input connector.

Example :_test:SGEN:PDAT1:INPut:DELAy:CYCL?
 :_test:SGEN1:PDAT1:TERM1:INPut:DELAy:CYCL?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DELAy:CYCL?
 might return:
 5.000000E-001

:INPut:DELay:TIME

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELay:TIME <Time>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELay:TIME <Time>
 :<Handle>[:CGROUP(*)]:MODule(*):CONNector(*):INPut:DELay:TIME <Time>

Parameters <Time> Delay in seconds.

If the delay is specified by :INPut:DELay:CYCLes and DELay:TIME, the corresponding delay will be calculated. The number of cycles is converted into seconds and added to the specified DELay:TIME value.

If :INPut:DELay is used, the value will be interpreted as a timing value only. Therefore, :INPut:DELay:CYCLes is set to zero.

Example :_test:SGEN:PDAT1:INPut:DELAY:TIME 5e-9
 :_test:SGEN1:PDAT1:TERM1:INPut:DELAY:TIME 5e-9
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DELAY:TIME 5e-9

:INPut:DELay:TIME?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELay:TIME?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELay:TIME?
 :<Handle>[:CGROUP(*)]:MODule(*):CONNector(*):INPut:DELay:TIME?

Return Value Returns the current additional delay value of the sampling edge for the specified analyzer input connector. When there is no CYCLe value specified, it corresponds to the DELay value.

Example :_test:SGEN:PDAT1:INPut:DELAY:TIME?
 :_test:SGEN1:PDAT1:TERM1:INPut:DELAY:TIME?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DELAY:TIME?
might return:
 5.000000E-009

:INPut:DELAy:ACTual?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELAy:ACTual?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELAy:ACTual?
 :<Handle>[:CGRoup(*)]:MODUle(*):CONNector(*):INPut:DELAy:ACTual?

Return Value The Agilent 81250 has the following methods to get the expected data and the incoming data aligned to ensure proper real-time compare:

- Synchronous measurement

The exact sample-point delay is well-known in advance and is programmed as the sample delay. In this case, the actual delay query returns:

ACT DELAY= Delay(Time) + Delay(Cycles) + Delay(Sweep)

- Auto delay adjust

The exact sample delay is not known in advance, but a certain delay range the correct sample point will be inside. The actual delay query returns:

ACT DELAY= Delay(Time) + Delay(Cycles) + Delay(Sweep) + Delay(B-SYNC)

- Auto Bit Synchronization

Not even a delay range is known within which the incoming data will start. The data can come at any time after the system is started. The actual delay query returns:

ACT DELAY= Delay(Time) + Delay(Cycles) + Delay(Sweep) + Delay(B-SYNC)

Note that the actual delay may exceed the returned value by a multiple the period.

Delay(Time), Delay(Cycles), and Delay(Sweep) are shown in property window of the user interface. To query the individual values, use “:INPut:DELAy:TIME?” on page 257, “:INPut:DELAy:CYCLes?” on page 256 and “:INPut:DELAy:SWEep?” on page 259.

Delay(B-SYNC) is the bit sync delay. It is measured by every analyzer involved and is reported to the firmware and added to the actual delay after successful synchronization.

Example :_test:SGEN:PDAT1:INPut:DELAy:ACT?
 :_test:SGEN1:PDAT1:TERM1:INPut:DELAy:ACT?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DELAy:ACT?

might return:

1.25E-9

:INPut:DELay:SWEep

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELay:SWEep <Sweep>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELay:SWEep <Sweep>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:DELay:SWEep
 <Sweep>

Parameters <Sweep> Sets the delay sweep value in the range of -1.0 to +1.0.

The delay sweep allows to shift the analyzer sampling point by up to ± 1 clock periods while a test is running. This makes it possible to measure the eye opening of a superimposed signal without interrupting the test.

The delay sweep is available on E4863A and E4865A frontends, and on E4835A frontends with a frequency higher than 20.8 MHz and highest possible segment resolution.

Example :_test:SGEN:PDAT1:INPut:DELAY:SWE -0.4
 :_test:SGEN:PDAT1:TERM1:INPut:DELAY:SWE 0.1
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DELAY:SWE 0.75

:INPut:DELay:SWEep?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DELay:SWEep?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DELay:SWEep?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:DELay:SWEep?

Return Value Returns the current delay sweep value in the range of -1.0 to +1.0.

Example :_test:SGEN:PDAT1:INPut:DELAY:SWE?
 :_test:SGEN:PDAT1:TERM1:INPut:DELAY:SWE?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DELAY:SWE?

might return:

-0.4

:INPut:TCONfig


Syntax :<Handle>:SGENeral:PDATa(*):INPut:TCONfig <VOLTag | DIFFerential>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:TCONfig
 <VOLTag | DIFFerential>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:TCONfig
 <VOLTag | DIFFerential>

Parameters <VOLTag | DIFFerential> Selects the termination model for input frontends:

- VOLTag selects termination via resistor against a termination voltage.
 If VOLTag is selected, the termination resistor and termination voltage can be set with “:INPut:IMPedance[:INTernal]” on page 252 and “:INPut:TVOLtage” on page 250.
- DIFFerential selects termination via a resistor against the complement input (DIFFerential is only supported for E4835A, E4863A and E4865A differential input frontends).
 If DIFFerential is selected, the differential termination resistor can be set with “:INPut:DIMPedance” on page 261.

Description For input frontends two possible termination models are available:

- Via a resistor against a termination voltage. The resistor might be high impedance or 50 Ohm. In the following picture this is shown for single ended and differential inputs.

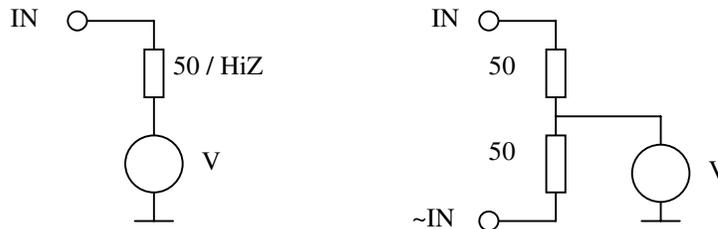

Example :_test:SGEN:PDAT1:INP:TCON DIFF
 :_test:SGEN:PDAT1:TERM1:INP:TCON DIFF
 :_test:MOD1:CONN2:INP:TCON VOLT

:INPut:TCONfig?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:TCONfig?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:TCONfig?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:TCONfig?

Return Value Returns the termination model for input frontends (see “:INPut:TCONfig” on page 260).

Example :_test:SGEN:PDAT1:TERM1:INP:TCON?
 :_test:SGEN1:PDAT1:TERM1:INPut:TCONFIG?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INP:TCON?
might return:
 DIFF

:INPut:DIMPedance

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DIMPedance[:INTernal] <Impedance>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DIMPedance[:INTernal]
 <Impedance>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:DIMPedance[:
 INTernal] <Impedance>

Parameters <Impedance> Sets the impedance between the IN and \IN\ inputs of a frontend when the differential termination model is selected (see “:INPut:TCONfig” on page 260).

The only possible value is 100 Ohm.

Example :_test:SGEN:PDAT:INP:DIMP 100
 :_test:SGEN:PDAT1:TERM1:INP:DIMP 100
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DIMP 100

:INPut:DIMPedance?

Syntax :<Handle>:SGENeral:PDATa(*):INPut:DIMPedance[:INTernal]?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):INPut:DIMPedance[:INTernal]?
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):INPut:DIMPedance[:
 INTernal]?

Return Value Returns the differential termination resistor (see “:INPut:TCONfig” on page 260).

The only possible value is 100 Ohm.

Example :_test:SGEN:PDAT:INP:DIMP?
 :_test:SGEN:PDAT1:TERM1:INP:DIMP?
 :_test:CGROUP1:MODULE2:CONNECTOR4:INPut:DIMP?
 might return:
 100

:INPut:DISConnect:MODE?

Syntax :<Handle>:CGRoup(*):MODule(*):CONNector(*):INPut:DISConnect:MODE?
 :<Handle>:SGENeral:PDATa(*):INPut:DISConnect:MODE?
 :<Handle>:SGENeral:PDATa(*):TERMinal:INPut:DISConnect:MODE?

Return Value Returns how the specified connector is to be disconnected when the SGENeral:GLOBal:CONNect OFF command is executed. Can be either RELay (disconnected by switching off the corresponding relay) or VOLtage (disconnected by reducing the voltage to 0).

Example :_test:CGR1:MOD1:CONN1:INP:DISC:MODE?
 might return:
 REL

:INPut:DISConnect:MODE

Syntax :<Handle>:CGRoup(*):MODule(*):CONNector(*):INPut:DISConnect:MODE
RELay|VOLTage
:<Handle>:SGENeral:PDATA(*):INPut:DISConnect:MODE RELay|VOLTage
:<Handle>:SGENeral:PDATA(*):TERMinal:INPut:DISConnect:MODE
RELay|VOLTage

Parameters **RELay** Disconnects the specified connector by switching the corresponding relay when the `SGENeral:GLOBal:CONNect OFF` command is executed.

VOLTage Disconnects the specified connector by setting the voltage to 0 when the `SGENeral:GLOBal:CONNect OFF` command is executed.

Example :_test:CGR1:MOD1:CONN1:INP:DISC:MODE REL

Optical Input Commands

The optical input commands are used for ParBERT optical analyzers, such as the E4811A. The following commands are available:

- **STATe**
Sets/returns the state of the O/E converter.
- **POWer:UNIT**
Sets/returns the unit used for the 0/1 decision threshold.
- **POWer:THReshold**
Sets/returns the 0/1 decision threshold.
- **MEASure**
Measures the average signal power and sets this as the 0/1 decision threshold.
- **DLCalibration**
Performs Dark Level Calibration.

See also “*Optical Output Commands*” on page 280.

:INPut:OPTic[:STATe][:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:[STATe]:[VALue] <OFF|ON>
 :<Handle>:SGENeral:PDATA(*):INPut:OPTic:[STATe]:[VALue] <OFF|ON>
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:[STATe]:[VALue] <OFF|ON>

Parameters <OFF|ON> Sets the state of the optical channel(s) when in optical mode. The electrical analyzer is automatically enabled/disabled.

Examples :_test:CGR1:MOD1:CONN1:INP:OPT:STAT:VAL OFF
 :_test:CGR1:MOD1:CONN1:INP:OPT OFF

:INPut:OPTic[:STATe][:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:[STATe]:[VALue]? <NFORce|FORCe>
 :<Handle>:SGENeral:PDATA(*):INPut:OPTic:[STATe]:[VALue]? <NFORce|FORCe>
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:[STATe]:[VALue]? <NFORce|FORCe>

Return Value The state of the optical channel(s) when in optical mode.

Parameters <NFORce|FORCe> Defines how the query is executed:

- NFORce
 Default value. Only the firmware is queried for the current state.
- FORCe
 When FORCe is entered, the firmware checks the current condition in the hardware. This is required to make sure that the optical channel's electrical interface is really switched on.

NOTE The FORCe query is slower than NFORce.

Examples :_test:CGR1:MOD1:CONN1:INP:OPT:STAT:VAL? FORC
 :_test:CGR1:MOD1:CONN1:INP:OPT?
might return:
 ON

:INPut:OPTic:POWer:UNIT[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:POWer:UNIT[:VALue] <WATT|DBM>

:<Handle>:SGENeral:PDATA(*):INPut:OPTic:POWer:UNIT[:VALue] <WATT|DBM>

:<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:POWer:UNIT[:VALue] <WATT|DBM>

Parameters <WATT|DBM> Selects the unit for the 0/1 decision threshold of the selected optical input port, terminal, or connector.

dBm is a unitless logarithmic alternative to Watt. The following calculations are used for transformations:

- $\text{Power}_{\text{dBm}} = 10 \cdot \log(\text{Power}_{\text{Watt}}/0.001 \text{ W})$
- $\text{Power}_{\text{dBm}} = 10 \cdot \log(\text{Power}_{\text{Watt}}/1 \text{ mW})$
- $\text{Power}_{\text{Watt}} = 1 \text{ mW} \cdot 10^{(\text{Power}_{\text{dBm}}/10)}$

Examples :_test:CGR1:MOD1:CONN1:INP:OPT:POW:UNIT:VAL WATT

:_test:CGR1:MOD1:CONN1:INP:OPT:POW:UNIT WATT

:INPut:OPTic:POWer:UNIT[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:POWer:UNIT[:VALue]?

:<Handle>:SGENeral:PDATA(*):INPut:OPTic:POWer:UNIT[:VALue]?

:<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:POWer:UNIT[:VALue]?

Return Value Used power unit for setting and querying the 0/1 decision threshold.

Examples :_test:CGR1:MOD1:CONN1:INP:OPT:POW:UNIT:VAL?

:_test:CGR1:MOD1:CONN1:INP:OPT:POW:UNIT?

might return:

WATT

:INPut:OPTic:POWer:THReshold[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:POWer:THReshold[:VALue] <DT>
 :<Handle>:SGENeral:PDATA(*):INPut:OPTic:POWer:THReshold[:VALue] <DT>
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:POWer:THReshold[:VALue] <DT>

Parameters <DT> 0/1 Decision Threshold for the comparator built into the O/E converter; signals above this value are treated as 1s, signals below this value are treated as 0s. The current unit can be queried with “:INPut:OPTic:POWer:UNIT[:VALue]?” on page 265.

:INPut:OPTic:POWer:THReshold[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:POWer:THReshold[:VALue]?
 :<Handle>:SGENeral:PDATA(*):INPut:OPTic:POWer:THReshold[:VALue]?
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:POWer:THReshold[:VALue]?

Return Value 0/1 decision threshold of the connector, port or terminal. The unit of the returned value can be queried with “:INPut:OPTic:POWer:UNIT[:VALue]?” on page 265

:INPut:OPTic:WAVelength[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:WAVelength[:VALue] <length>
 :<Handle>:SGENeral:PDATA(*):INPut:OPTic:WAVelength[:VALue] <length>
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:WAVelength[:VALue] <length>

Parameters <length> Standard calibration wavelength for the corresponding port, terminal or connector in meters. This command is only valid for the E4811A module, and only if this has been ordered with special calibration options for different wavelength requirements.

The standard calibration for 850nm is included in all of the special calibration options. Depending on the ordered calibration, one or more additional wavelength settings might be available. Note that

loading of settings can fail if the setting selects a wavelength that is not available for the system that loads the setting.

Example `cgr:mod3:conn:inp:opt:wav 850e-9`

:INPut:OPTic:WAVelength[:VALue]?

Syntax `:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:WAVelength[:VALue]?`
`:<Handle>:SGENeral:PDATA(*):INPut:OPTic:WAVelength[:VALue]?`
`:<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:WAVelength[:VALue]?`

Return Value Returns the standard calibration wavelength in nanometer for the specified port, terminal, or connector. This query is only valid for the E4811A module, and only if this has been ordered with special calibration options for different wavelength requirements.

Example `cgr:mod3:conn:inp:opt:wav?`

might return:

`8.50e-7`

:INPut:OPTic:MEASure

Syntax `:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:MEASure`
`:<Handle>:SGENeral:PDATA(*):INPut:OPTic:MEASure`
`:<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:MEASure`

Measures the average signal power and sets this as the 0/1 decision threshold.

Examples `:_test:CGR1:MOD1:CONN1:INP:OPT:MEAS`

`:_test:CGR1:MOD1:CONN1:INP:OPT:MEAS`

:INPut:OPTic:DLCalibration

Syntax `:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):INPut:OPTic:DLCalibration`
`:<Handle>:SGENeral:PDATA(*):INPut:OPTic:DLCalibration`
`:<Handle>:SGENeral:PDATA(*):TERMinal(*):INPut:OPTic:DLCalibration`

Performs **Dark Level Calibration** on the port, terminal, or connector. For more information on Dark Level Calibration, see *How to Set Optical Analyzer Levels* in the *ParBERT System User Guide*.

It is recommended to perform Dark Level Calibration after the ParBERT has completely warmed up (~30 minutes), or after the temperature has changed by more than 10 °C (18 °F).

Output Parameter Commands

The commands for specifying the output parameters are available on port, terminal and connector level. The parameters can be specified separately for pulse and data ports.

For optical modules, see “*Optical Output Commands*” on page 280 for the commands.

:OUTPut[:STATe]

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut[:STATe] <ON | OFF>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut[:STATe] <ON | OFF>
 :<Handle>:SGENeral:PPULse(*):OUTPut[:STATe] <ON | OFF>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut[:STATe] <ON | OFF>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut[:STATe] <ON | OFF>

Parameters <ON | OFF> Switch the normal connector ON or OFF.

Controls whether the output connectors are open (ON) or closed (OFF).

Example :_test:SGEN:PDAT1:OUTP ON
 :_test:SGEN:PDAT1:TERM1:OUTP:STAT ON
 :_test:SGEN:PPUL1:OUTP ON
 :_test:SGEN:PPUL1:TERM1:OUTP:STAT OFF
 :_test:MOD2:CONN1:OUTP OFF

:OUTPut[:STATe]?

Syntax :<Handle>:SGENeral:PDATa(*)**:OUTPut**[:STATe]? <NFORce|FORCe>
 :<Handle>:SGENeral:PDATa(*)**:TERMinal**(*)**:OUTPut**[:STATe]?
 <NFORce|FORCe>
 :<Handle>:SGENeral:PPULse(*)**:OUTPut**[:STATe]? <NFORce|FORCe>
 :<Handle>:SGENeral:PPULse(*)**:TERMinal**(*)**:OUTPut**[:STATe]?
 <NFORce|FORCe>
 :<Handle>[:CGRoup(*)]:MODule(*)**:CONNector**(*)**:OUTPut**[:STATe]?
 <NFORce|FORCe>

Parameters <NFORce|FORCe> Defines how the query is executed:

- NFORce

Default value. Only the firmware is queried for the current state.

- FORCe

When FORCe is entered, the firmware checks the current condition in the hardware. This is required to make sure that the output is really switched on, or to check if the protection circuit within the output has turned off the channel to protect it from damage.

NOTE The FORCe call is slower than NFORce.

Return Value Returns the current connection state for the specified output connectors.

```
:_test:SGEN:PDAT1:OUTP? NFOR
:_test:SGEN:PDAT1:TERM1:OUTP:STAT? FORC
:_test:SGEN:PPUL1:OUTP? NFOR
:_test:SGEN:PPUL1:TERM1:OUTP:STAT? FORC
:_test:MOD2:CONN1:OUTP?
```

might return:

ON

:OUTPut:POLarity

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:POLarity <NORMal | INVerted>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:POLarity
 <NORMal | INVerted>
 :<Handle>:SGENeral:PPULse(*):OUTPut:POLarity <NORMal | INVerted>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:POLarity
 <NORMal | INVerted>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:POLarity
 <NORMal | INVerted>

Parameters <NORMal | INVerted> Sets the output polarity to either normal or inverted (NORMal is the reset value).

This command is not supported for E4863A and E4865A frontends.

Example :_test:SGEN:PDAT1:OUTP:POL NORM
 :_test:SGEN:PDAT1:TERM1:OUTP:POL INV
 :_test:SGEN:PPUL1:OUTP:POL NORM
 :_test:SGEN:PPUL1:TERM1:OUTP:POL NORM
 :_test:CGR1:MOD2:CONN4:OUTP:POL INV

:OUTPut:POLarity?

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:POLarity?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:POLarity?
 :<Handle>:SGENeral:PPULse(*):OUTPut:POLarity?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:POLarity?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:POLarity?

Return Value Returns the current output polarity (NORMal or INVerted).

Example :_test:SGEN:PDAT1:OUTP:POL?
 :_test:SGEN:PDAT1:TERM1:OUTP:POL?
 :_test:SGEN:PPUL1:OUTP:POL?
 :_test:SGEN:PPUL1:TERM1:OUTP:POL?
 :_test:CGR1:MOD2:CONN4:OUTP:POL?

might return:

NORM

:OUTPut:CStAtE

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:CStAtE <ON | OFF>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:CStAtE <ON | OFF>
 :<Handle>:SGENeral:PPULse(*):OUTPut:CStAtE <ON | OFF>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:CStAtE <ON | OFF>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:CStAtE <ON | OFF>

Parameters <ON | OFF> Switches the complement connector ON or OFF.

Controls whether the complement output connectors are open (ON) or closed (OFF).

Example :_test:SGEN:PDAT1:OUTP:CST ON
 :_test:SGEN:PDAT1:TERM1:OUTP:CSTAT OFF
 :_test:SGEN:PPUL1:OUTP:CST ON
 :_test:SGEN:PPUL1:TERM1:OUTP:CSTAT OFF
 :_test:CGR1:MOD2:CONN2:OUTP:CSTAT ON

:OUTPut:CStAtE?

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:CStAtE?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:CStAtE?
 :<Handle>:SGENeral:PPULse(*):OUTPut:CStAtE?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:CStAtE?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:CStAtE?

Return Value Returns the current connection state (enabled or disabled) for the complement connectors of the specified port, terminal, or connector.

Example :_test:SGEN:PDAT1:OUTP:CST?
 :_test:SGEN:PDAT1:TERM1:OUTP:CSTAT?
 :_test:SGEN:PPUL1:OUTP:CST?
 :_test:SGEN:PPUL1:TERM1:OUTP:CSTAT?
 :_test:CGR1:MOD2:CONN2:OUTP:CSTAT?

might return:

OFF

:OUTPut:TVOLtage

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:TVOLtage <TerminationVoltage>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:TVOLtage
 <TerminationVoltage>
 :<Handle>:SGENeral:PPULse(*):OUTPut:TVOLtage <TerminationVoltage>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:TVOLtage
 <TerminationVoltage>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:TVOLtage
 <TerminationVoltage>

Parameters <TerminationVoltage> Termination voltage (<NRf>).
 Sets the external termination voltage, default is 0 volts = ground.
 Valid range is -2.0 to +3.0 volts.

Example :_test:SGEN:PDAT1:OUTP:TVOLT -1
 :_test:SGEN:PDAT1:TERM1:OUTP:TVOL 2.0
 :_test:SGEN:PPUL1:OUTP:TVOLT -1
 :_test:SGEN:PPUL1:TERM1:OUTP:TVOL 2.0
 :_test:CGROUP1:MODULE2:CONNECTOR4:OUTPUT:TVOLTAGE -1

:OUTPut:TVOLtage?

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:TVOLtage?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:TVOLtage?
 :<Handle>:SGENeral:PPULse(*):OUTPut:TVOLtage?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:TVOLtage?
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:TVOLtage?

Return Value Returns the currently set value for the external Termination VOLTage.

Example :_test:SGEN:PDAT1:OUTP:TVOLT?
 :_test:SGEN:PDAT1:TERM1:OUTP:TVOL?
 :_test:SGEN:PPUL1:OUTP:TVOLT?
 :_test:SGEN:PPUL1:TERM1:OUTP:TVOL?
 :_test:CGROUP1:MODULE2:CONNECTOR4:OUTPUT:TVOLTAGE?

might return:

-1

:OUTPut:IMPedance:EXTernal

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:IMPedance:EXTernal
<LoadImpedance>
:<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:IMPedance:EXTernal
<LoadImpedance>
:<Handle>:SGENeral:PPULse(*):OUTPut:IMPedance:EXTernal
<LoadImpedance>
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:IMPedance:EXTernal
<LoadImpedance>
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:IMPedance:
EXTernal <LoadImpedance>

Parameters <LoadImpedance> Impedance of the DUT (load) in Ohms (<NRf>).
Sets the external termination impedance, this is the real load
impedance of the DUT.
Any negative value is interpreted as “into open”.

Example :_test:SGEN:PDAT1:OUTP:IMP:EXT 500
:_test:SGEN:PDAT1:TERM1:OUTP:IMP:EXT 70
:_test:SGEN:PPUL1:OUTP:IMP:EXT 500
:_test:SGEN:PPUL1:TERM1:OUTP:IMP:EXT 70
:_test:MOD2:CONN3:OUTP:IMP:EXT 500

:OUTPut:IMPedance:EXTernal?

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:IMPedance:EXTernal?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:IMPedance:EXTernal?
:<Handle>:SGENeral:PPULse(*):OUTPut:IMPedance:EXTernal?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:IMPedance:EXTernal?
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:IMPedance:
EXTernal?

Return Value Returns the currently set value for the termination (load) impedance.

Example :_test:SGEN:PDAT1:OUTP:IMP:EXT?
:_test:SGEN:PDAT1:TERM1:OUTP:IMP:EXT?
:_test:SGEN:PPUL1:OUTP:IMP:EXT?
:_test:MOD2:CONN3:OUTP:IMP:EXT?
might return:
500

:OUTPut:TCONfig


Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:TCONfig <VOLTag | DIFFerential>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:TCONfig
 <VOLTag | DIFFerential>
 :<Handle>:SGENeral:PPULse(*):OUTPut:TCONfig <VOLTag | DIFFerential>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:TCONfig
 <VOLTag | DIFFerential>
 :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:TCONfig
 <VOLTag | DIFFerential>

Parameters <VOLTag | DIFFerential> Selects the termination model for output frontends:


- VOLTag selects termination via resistor against a termination voltage (this is the reset value).
 If VOLTag is selected, the termination resistor and termination voltage can be set with “:OUTPut:IMPedance:EXTernal” on page 273 and “:OUTPut:TVOLtage” on page 272.
- DIFFerential selects termination via a resistor against the complement output.
 If DIFFerential is selected, the differential termination resistor can be set with “:OUTPut:DIMPedance:EXTernal” on page 276.

Description For output frontends, it is necessary to specify how the signal will be terminated. There are two possible termination models available:

- Via a resistor against a termination voltage; the resistor might be high impedance. Optimum signal performance is achieved with 50 Ohm. In the following picture, this is shown for single ended and differential outputs.

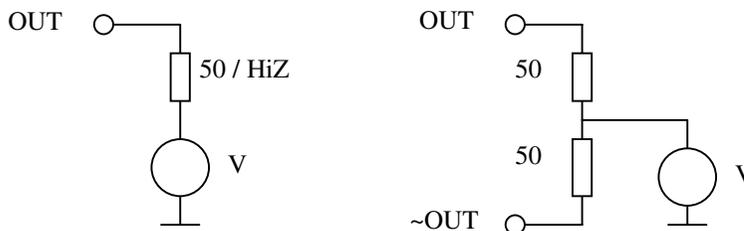

- Via a resistor to the complement output. Optimum signal performance is achieved with 100 Ohms.



Example

```

:_test:SGEN:PDAT1:OUTP:TCON DIFF
:_test:SGEN:PDAT1:TERM1:OUTP:TCON DIFF
:_test:SGEN:PPUL1:OUTP:TCON VOLT
:_test:SGEN:PPUL1:TERM1:OUTP:TCON DIFF
:_test:MOD2:CONN3:OUTP:TCON VOLT

```

:OUTPut:TCONfig?

Syntax

```

:<Handle>:SGENeral:PDATa(*):OUTPut:TCONfig?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:TCONfig?
:<Handle>:SGENeral:PPULse(*):OUTPut:TCONfig?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:TCONfig?
:<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:TCONfig?

```

Return Value Returns the termination model for output frontends (see “:OUTPut:TCONfig” on page 274).

Example

```

:_test:SGEN:PDAT1:OUTP:TCON?
:_test:SGEN:PDAT1:TERM1:OUTP:TCON?
:_test:SGEN:PPUL1:OUTP:TCON?
:_test:SGEN:PPUL1:TERM1:OUTP:TCON?
:_test:MOD2:CONN3:OUTP:TCON?

```

might return:

DIFF

:OUTPut:DIMPedance:EXTernal

Syntax SGENeral:PDATa(*):OUTPut:DIMPedance:EXTernal <Impedance>
 SGENeral:PDATa(*):TERMinal(*):OUTPut:DIMPedance:EXTernal
 <Impedance>
 SGENeral:PPULse(*):OUTPut:DIMPedance:EXTernal <Impedance>
 SGENeral:PPULse(*):TERMinal(*):OUTPut:DIMPedance:EXTernal
 <Impedance>
 CGR(*):MOD(*):CONNector(*):OUTP:DIMP:EXT <Impedance>

Parameters <Impedance> Sets the impedance between the OUT and \OUT\
 output frontend when the differential termination model is selected
 (see “:OUTPut:TCONfig” on page 274).

Usually 100 Ohms are used for termination.

Example :_test:SGEN:PDAT:OUTP:DIMP:EXT 100
 :_test:SGEN:PDAT1:TERM2:OUTP:DIMP:EXT 50
 :_test:SGEN:PPUL:OUTP:DIMP:EXT 100
 :_test:SGEN:PPUL2:TERM3:OUTP:DIMP:EXT 100

:OUTPut:DIMPedance:EXTernal?

Syntax SGENeral:PDATa(*):OUTPut:DIMPedance:EXTernal?
 SGENeral:PDATa(*):TERMinal(*):OUTPut:DIMPedance:EXTernal?
 SGENeral:PPULse(*):OUTPut:DIMPedance:EXTernal?
 SGENeral:PPULse(*):TERMinal(*):OUTPut:DIMPedance:EXTernal?
 CGRoup(*):MODule(*):CONNector(*):OUTPut:DIMPedance:EXTernal?

Return Value Returns the differential termination resistor (see “:OUTPut:TCONfig”
 on page 274).

Example :_test:SGEN:PDAT:OUTP:DIMP:EXT?
 :_test:SGEN:PDAT1:TERM2:OUTP:DIMP:EXT?
 :_test:SGEN:PPUL:OUTP:DIMP:EXT?
 :_test:SGEN:PPUL2:TERM3:OUTP:DIMP:EXT?
 :_test:MOD2:CONN3:OUTP:DIMP:EXT?

might return:

100

:OUTPut:CAConfiguration[:MODE]

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:CAConfiguration[:MODE] <OFF | D2 | D4 | A2>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:CAConfiguration[:MODE] <OFF | D2 | D4 | A2>
 :<Handle>:SGENeral:PPULse(*):OUTPut:CAConfiguration[:MODE] <OFF | D2 | D4 | A2>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:CAConfiguration[:MODE] <OFF | D2 | D4 | A2>
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):OUTPut:CAConfiguration[:MODE] <OFF | D2 | D4 | A2>

Parameters <OFF | D2 | D4 | A2> Selects the channel-add mode of a port/terminal/ connector. The following modes are available:

- OFF (no channel addition). This is the reset value.
- D2 is a digital add of two channels (XOR). It can be used on the second and fourth frontend slot of an E4832A module if output frontends are plugged into this slot and into the one immediately above.
- D4 is a digital add of four channels (XOR). It can be used on the fourth frontend slot of an E4832A module if the whole module is equipped with output frontends.
- A2 is an analog add available only for E4838A frontends. It can be used on the second and fourth frontend slots of an E4832A module if an E4838A frontend is fitted there.

If A2 Mode is selected, the parameters specified by the following commands are additionally available:

- “:VOLTage[:LEVel][:IMMEDIATE]:CAConfiguration:LOW” on page 229
- “:PULSe:TRANsition:CAConfiguration[:LEADing]” on page 197
- “:PULSe:TRANsition:CAConfiguration:TRAILing” on page 199

Example :_test:SGEN:PDAT1:OUTP:CAC D2
 :_test:SGEN:PDAT1:TERM1:OUTP:CAC:MODE D4
 :_test:SGEN:PPUL1:OUTP:CAC D2
 :_test:SGEN:PPUL1:TERM1:OUTP:IMP:CAC:MODE D4
 :_test:cgr1:mod2:conn4:outp:cac A2

:OUTPut:CAConfiguration[:MODE]?

Syntax :<Handle>:SGENeral:PDATa(*):OUTPut:CAConfiguration[:MODE]?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:CAConfiguration[:MODE]?
 :<Handle>:SGENeral:PPULse(*):OUTPut:CAConfiguration[:MODE]?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:CAConfiguration[:MODE]?
 :<Handle>[:CGRoup(*):MODule(*):CONNector(*):OUTPut:CAConfiguration[:MODE]?

Return Value Returns the current channel addition mode of the specified port/terminal/connector.

Example :_test:SGEN:PDAT1:OUTP:CAC?
 :_test:SGEN:PDAT1:TERM1:OUTP:CAC:MODE?
 :_test:SGEN:PPUL1:OUTP:CAC?
 :_test:SGEN:PPUL1:TERM1:OUTP:CAC:MODE?
 :_test:cgr1:mod2:conn4:outp:cac?
 might return:
 D2

:OUTPut:DISConnect:MODE?

Syntax :<Handle>:CGRoup*:MODule*:CONNector*:OUTPut:DISConnect:MODE RELay|VOLTage
 :<Handle>:SGENeral:PDATa*:OUTPut:DISConnect:MODE RELay|VOLTage
 :<Handle>:SGENeral:PDATa*:TERMinal:OUTPut:DISConnect:MODE RELay|VOLTage
 :<Handle>:SGENeral:PPULse*:OUTPut:DISConnect:MODE RELay|VOLTage
 :<Handle>:SGENeral:PPULse*:TERMinal:OUTPut:DISConnect:MODE RELay|VOLTage

Return Value Returns how the specified connector is to be disconnected when the SGENeral:GLOBal:CONNect OFF command is executed. Can be either RELay (disconnected by switching off the corresponding relay) or VOLTage (disconnected by reducing the voltage to 0).

Example :_test:CGR1:MOD1:CONN1:OUTP:DISC:MODE?
 might return:
 REL

:OUTPut:DISConnect:MODE

Syntax :<Handle>:CGRoup*:MODUle*:CONNector*:OUTPut:DISConnect:MODE
RELay|VOLTage
:<Handle>:SGENeral:PDATA*:OUTPut:DISConnect:MODE RELay|VOLTage
:<Handle>:SGENeral:PDATA*:TERMinal:OUTPut:DISConnect:MODE
RELay|VOLTage
:<Handle>:SGENeral:PPULse*:OUTPut:DISConnect:MODE RELay|VOLTage
:<Handle>:SGENeral:PPULse*:TERMinal:OUTPut:DISConnect:MODE
RELay|VOLTage

Parameters <RELay|VOLTage> Sets how the connector, terminal or port is to be disconnected when the SGENeral:GLOBal:CONNect OFF command is executed:

- RELay
Disconnects the specified connector by switching the corresponding relay.
- VOLTage
Disconnects the specified connector by setting the voltage to 0.


Example :_test:CGR1:MOD1:CONN1:OUTP:DISC:MODE VOLT

Optical Output Commands

The optical output commands are used for ParBERT optical generators, such as the E4810A. The following commands are available:

- **STATe**
Sets/returns the state of the connector, terminal, or port.
- **METHod**
Sets/returns the state of the connector, terminal, or port.
- **POWER:UNIT**
- **Optical Power Parameters**

The following parameters are used for the optical power:

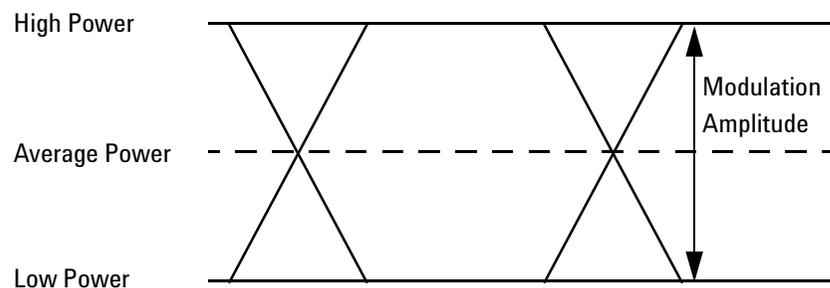

Not shown: Extinction ratio (\sim High/Low).

There are three possibilities of defining the optical waveform:

- Define the high and low power (**HIGH_LOW** method)
- Define the average power and the modulation amplitude (**AVER_MAMP** method)
- Define the average power and the extinction ratio (**AVER_ERAT** method)

The following table shows the relationship between the :OUTPut:OPTic:METhod parameter and the commands for setting the power levels:

Parameters	:OUTPut:OPTic:METhod		
	AVER_ERAT	AVER_MAMP	HIGH_LOW
High	Calculated	Calculated	Direct entry
Low	Calculated	Calculated	Direct entry
Average	Direct entry	Direct entry	Calculated
Modulation Amplitude	Calculated	Direct entry	Calculated
Extinction Ratio	Direct entry	Calculated	Calculated

The parameters are calculated as follows (based on the High and Low power values). Note that all powers are given in Watt.

- Average Power = (High + Low)/2
- Modulation Amplitude = High - Low
- Extinction Ratio_{None} = High/Low
- Extinction Ratio_{dB} = 10*log(High/Low)

See also “*Optical Input Commands*” on page 263.

:OUTPut:OPTic[:STATe][:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:[STATe]:[VALue] <OFF|ON>
 :<Handle>:SGENeral:PDATa(*):OUTPut:OPTic:[STATe]:[VALue] <OFF|ON>
 :<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:[STATe]:[VALue] <OFF|ON>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:OPTic:[STATe]:[VALue] <OFF|ON>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:[STATe]:[VALue] <OFF|ON>

Parameters <OFF|ON> Enables/disables the laser on the E/O converter. The electrical board is enabled/disabled automatically if the connector species is set to OPT.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:STAT:VAL OFF
 :_test:CGR1:MOD1:CONN1:OUTP:OPT OFF

:OUTPut:OPTic[:STATe][:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:[STATe]:[VALue]? <NFORce|FORCe>
 :<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:[STATe]:[VALue]?
 <NFORce|FORCe>
 :<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:[STATe]:[VALue]?
 <NFORce|FORCe>
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:[STATe]:[VALue]?
 <NFORce|FORCe>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:[STATe]:[VALue]?
 <NFORce|FORCe>

Return Value The state of the laser on the E/O converter.

Parameters <NFORce|FORCe> Defines how the query is executed:

- NFORce
 Default value. Only the firmware is queried for the current state.
- FORCe
 When FORCe is entered, the firmware checks the current condition in the hardware. This is required to make sure that the output is really switched on, or to check if the protection circuit within the output has turned off the channel to protect it from damage.

NOTE The FORCe query is slower than NFORce.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:STAT:VAL?
 :_test:CGR1:MOD1:CONN1:OUTP:OPT?
might return:
 ON

:OUTPut:OPTic:METHod[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:METHod:
[VALue] <AVER_ERAT | AVER_MAMP | HIGH_LOW>
:<Handle>:SGENeral:PDATa(*):OUTPut:OPTic:METHod:[VALue] <AVER_ERAT
| AVER_MAMP | HIGH_LOW>
:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:METHod:[VALue]
<AVER_ERAT | AVER_MAMP | HIGH_LOW>
:<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:OPTic:METHod:[VALue]
<AVER_ERAT | AVER_MAMP | HIGH_LOW>
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:METHod:[VALue]
<AVER_ERAT | AVER_MAMP | HIGH_LOW>

Parameters <AVER_ERAT | AVER_MAMP | HIGH_LOW> Sets the method used to define the optical levels:

- AVER_ERAT (Average Power / Extinction Ratio)
- AVER_MAMP (Average Power / Modulation Amplitude)
- HIGH_LOW (High Power / Low Power)

The optical parameters can always be queried, but only the parameters specified by METHod can be set. For example, if the METHod is AVER_MAMP, only average power and modulation amplitude can be directly set. Trying to set high power in this case results in an error.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:METH HIGH_LOW
:_test:CGR1:MOD1:CONN1:OUTP:OPT:UNIT WATT
:_test:CGR1:MOD1:CONN1:OUTP:OPT:HIGH 0.865242735174E-3

:OUTPut:OPTic:METHod[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:METHod:
[VALue]?
:<Handle>:SGENeral:PDATa(*):OUTPut:OPTic:METHod:[VALue]?
:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:METHod:[VALue]?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:OPTic:METHod:[VALue]?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:METHod:
[VALue]?

Return Value Returns the method used to set the optical levels:

- AVER_ERAT (Average Power / Extinction Ratio)
- AVER_MAMP (Average Power / Modulation Amplitude)
- HIGH_LOW (High Power / Low Power)

:OUTPut:OPTic:POWer:UNIT[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:UNIT:
[VALue] <WATT|DBM>
:<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:POWer:UNIT:[VALue]
<WATT|DBM>
:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:UNIT:[VALue]
<WATT|DBM>
:<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:POWer:UNIT:
[VALue] <WATT|DBM>
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:UNIT:
[VALue] <WATT|DBM>

Parameters <WATT|DBM> Selects the unit for all power parameters of the selected optical output port or terminal.

dBm is a unitless logarithmic alternative to Watt. The following calculations are used for transformations:

- $\text{Power}_{\text{dBm}} = 10 \cdot \log(\text{Power}_{\text{Watt}} / 0.001 \text{ W})$
- $\text{Power}_{\text{dBm}} = 10 \cdot \log(\text{Power}_{\text{Watt}} / 1 \text{ mW})$
- $\text{Power}_{\text{Watt}} = 1 \text{ mW} \cdot 10^{(\text{Power}_{\text{dBm}} / 10)}$

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT:VAL WATT
:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT WATT

:OUTPut:OPTic:POWer:UNIT[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:UNIT:
[VALue]?
:<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:POWer:UNIT:[VALue]?
:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:UNIT:[VALue]?
:<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:POWer:UNIT:
[VALue]?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:UNIT:
[VALue]?

Return Value Used power unit for setting and querying the optical power parameters.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT:VAL?
:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT?
might return:

WATT

:OUTPut:OPTic:POWer:AVERage[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:AVERage[:VALue] <avg. power>
 :<Handle>:SGENeral:PDATa(*):OUTPut:OPTic:POWer:AVERage[:VALue] <avg. power>
 :<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:AVERage[:VALue] <avg. power>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:OPTic:POWer:AVERage[:VALue] <avg. power>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:AVERage[:VALue] <avg. power>

Parameters <avg. power> Average power of the selected connector, terminal, or port.

NOTE When setting this parameter, the parameter defined by :OUTPut:OPTic:POW:UNIT is used.

This command can also only be used when the :OUTPut:OPTic:METHOD command is set appropriately.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:METH:VAL AVER_ERAT
 :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT:VAL WATT
 :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:AVER:VAL 0.501187233627E-3
 :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:METH AVER_MAMP
 :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT WATT
 :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:AVER 0.501187233627E-3

:OUTPut:OPTic:POWer:AVERage[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:AVERage[:VALue] ?
 :<Handle>:SGENeral:PDATa(*):OUTPut:OPTic:POWer:AVERage[:VALue] ?
 :<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:AVERage[:VALue] ?
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:OPTic:POWer:AVERage[:VALue] ?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:AVERage[:VALue] ?

Return Value Average power of the selected connector, terminal, or port.

Examples `:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:AVER:VAL?`
 `:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:AVER?`
might return:
 0.501187233627E-3

:OUTPut:OPTic:POWer:MAMPlitude[:VALue]

Syntax `:<Handle>[:CGROUP(*):MODULE(*):CONNECTOR(*):OUTPut:OPTic:POWer:MAMPlitude[:VALue] <mod. ampl.>`
 `:<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:POWer:MAMPlitude[:VALue] <mod. ampl.>`
 `:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:MAMPlitude[:VALue] <mod. ampl.>`
 `:<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:POWer:MAMPlitude[:VALue] <mod. ampl.>`
 `:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:MAMPlitude[:VALue] <mod. ampl.>`

Parameters **<mod. ampl.>** Modulation amplitude of the selected connector, terminal, or port.

NOTE When setting this parameter, the parameter defined by `:OUTPut:OPTic:POW:UNIT` is used.

This command can also only be used when the `:OUTPut:OPTic:METHOD` command is set appropriately.

Examples `:_test:CGR1:MOD1:CONN1:OUTP:OPT:METH DBM`
 `:_test:CGR1:MOD1:CONN1:OUTP:OPT:MAMP -1.37802405912`

:OUTPut:OPTic:POWer:MAMPlitude[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:MAMPlitude:[VALue]?

:<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:POWer:MAMPlitude:[VALue]?

:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:MAMPlitude:[VALue]?

:<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:POWer:MAMPlitude:[VALue]?

:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:MAMPlitude:[VALue]?

Return Value Modulation amplitude of the selected connector, terminal, or port.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:MAMP?

:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:MAMP:VAL?

might return:

-1.37802405912

:OUTPut:OPTic:POWer:HIGh[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:HIGh:[VALue] <high power>

:<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:POWer:HIGh:[VALue] <high power>

:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:HIGh:[VALue] <high power>

:<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:POWer:HIGh:[VALue] <high power>

:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:HIGh:[VALue] <high power>

Parameters <high power> High power of the selected connector, terminal, or port.

NOTE When setting this parameter, the parameter defined by :OUTPut:OPTic:POW:UNIT is used.

This command can also only be used when the :OUTPut:OPTic:METHOD command is set appropriately.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT DBM

:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:HIGh -0.628620384795

:OUTPut:OPTic:POWer:HIGH[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:HIGH:
[VALue]?
:<Handle>:SGENeral:PDATA(*) :OUTPut:OPTic:POWer:HIGH:[VALue]?
:<Handle>:SGENeral:PPULse(*) :OUTPut:OPTic:POWer:HIGH:[VALue]?
:<Handle>:SGENeral:PDATA(*) :TERMinal(*) :OUTPut:OPTic:POWer:HIGH:
[VALue]?
:<Handle>:SGENeral:PPULse(*) :TERMinal(*) :OUTPut:OPTic:POWer:HIGH:
[VALue]?

Return Value High power of the selected connector, terminal, or port.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:HIGH?
:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:HIGH:VAL?
might return:
-0.628620384795

:OUTPut:OPTic:POWer:LOW[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:LOW:
[VALue] <low power>
:<Handle>:SGENeral:PDATA(*) :OUTPut:OPTic:POWer:LOW:[VALue] <low
power>
:<Handle>:SGENeral:PPULse(*) :OUTPut:OPTic:POWer:LOW:[VALue] <low
power>
:<Handle>:SGENeral:PDATA(*) :TERMinal(*) :OUTPut:OPTic:POWer:LOW:
[VALue] <low power>
:<Handle>:SGENeral:PPULse(*) :TERMinal(*) :OUTPut:OPTic:POWer:LOW:
[VALue] <low power>

Parameters <low power> Low power of the selected connector, terminal, or port.

NOTE When setting this parameter, the parameter defined by :OUTPut:OPTic:POW:UNIT is used.

This command can also only be used when the :OUTPut:OPTic:METHOD command is set appropriately.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:UNIT DBM
:_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:LOW -8.6286203848

:OUTPut:OPTic:POWer:LOW[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:POWer:LOW:
[VALue]?
:<Handle>:SGENeral:PDATa(*):OUTPut:OPTic:POWer:LOW:[VALue]?
:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:POWer:LOW:[VALue]?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:OPTic:POWer:LOW:
[VALue] <low power>
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:POWer:LOW:
[VALue] <low power>

Return Value Low power of the selected connector, terminal, or port.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:POW:LOW?
might return:
-8.6286203848

:OUTPut:OPTic:ERATio[:VALue]

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:ERATio:
[VALue] <ext. ratio>
:<Handle>:SGENeral:PDATa(*):OUTPut:OPTic:ERATio:[VALue] <ext. ratio>
:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:ERATio:[VALue] <ext. ratio>
:<Handle>:SGENeral:PDATa(*):TERMinal(*):OUTPut:OPTic:ERATio:[VALue]
<ext. ratio>
:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:ERATio:[VALue]
<ext. ratio>

Parameters <ext. ratio> Extinction ratio of the selected connector, terminal, or port.

NOTE When setting this parameter, the parameter defined by :OUTPut:OPTic:POW:ERAT:UNIT is used.

This command can also only be used when the :OUTPut:OPTic:METHOD command is set appropriately.

Examples :_test:CGR1:MOD1:CONN1:OUTP:OPT:ERAT 8
:_test:CGR1:MOD1:CONN1:OUTP:OPT:ERAT:VAL 8

:OUTPut:OPTic:ERATio[:VALue]?

- Syntax** :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:ERATio:
[VALue]?
- :<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:ERATio:[VALue]?
- :<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:ERATio:[VALue]?
- :<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:ERATio:[VALue]?
- :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:ERATio:[VALue]?
- Return Value** Extinction ratio of the selected connector, terminal, or port according to :OUTPut:OPTic:ERATio:UNIT.

- Examples** :_test:CGR1:MOD1:CONN1:OUTP:OPT:ERAT?
- :_test:CGR1:MOD1:CONN1:OUTP:OPT:ERAT:VAL?
- might return:
- 8.0E+0

:OUTPut:OPTic:ERATio:UNIT[:VALue]

- Syntax** :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:ERATio:
UNIT:[VALue] <NONE|DB>
- :<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:ERATio:UNIT:[VALue]
<NONE|DB>
- :<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:ERATio:UNIT:[VALue]
<NONE|DB>
- :<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:ERATio:[VALue]
<NONE|DB>
- :<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:ERATio:[VALue]
<NONE|DB>
- Parameters** <NONE|DB> Selects the unit for the extinction ratio of the selected optical connector, port, or terminal.
- NONE (linear value used)
 - DB (logarithmic value used)

- Example** :_test:CGR1:MOD1:CONN1:OUTP:OPT:UNIT DB
- :_test:CGR1:MOD1:CONN1:OUTP:OPT:UNIT:VAL DB

:OUTPut:OPTic:ERATio:UNIT[:VALue]?

Syntax :<Handle>[:CGRoup(*)]:MODule(*):CONNector(*):OUTPut:OPTic:ERATio:UNIT[:VALue]?

:<Handle>:SGENeral:PDATA(*):OUTPut:OPTic:ERATio:UNIT[:VALue]?

:<Handle>:SGENeral:PPULse(*):OUTPut:OPTic:ERATio:UNIT[:VALue]?

:<Handle>:SGENeral:PDATA(*):TERMinal(*):OUTPut:OPTic:ERATio:UNIT[:VALue]?

:<Handle>:SGENeral:PPULse(*):TERMinal(*):OUTPut:OPTic:ERATio:UNIT[:VALue]?

Return Value Unit used for the extinction ratio of the selected optical connector, port, or terminal. Can be:

- NONE (linear value used)
- DB (logarithmic value used)

Example :_test:CGR1:MOD1:CONN1:OUTP:OPT:UNIT?

:_test:CGR1:MOD1:CONN1:OUTP:OPT:UNIT:VAL?

might return:

DB

Clock Output Commands

The clock output commands to control the N4872/74's clock output signal. Correction factors can also be applied to the clock signal's amplitude and offset; see also "*Amplitude/Offset Correction Factor Commands*" on page 234

:CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH <NRf>
 :<Handle>:SGENERAL:PDATa(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH <NRf>
 :<Handle>:SGENERAL:PDATa(*):TERMINAL(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH <NRf>

Parameters <NRf> The upper voltage level of the N4872/74's clock output signal.

Example :_test:cgr:mod2:conn:volt:high 1.2

:CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH?

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH?
 :<Handle>:SGENERAL:PDATa(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH?
 :<Handle>:SGENERAL:PDATa(*):TERMINAL(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:HIGH?

Return Value Returns the upper voltage level of the N4872/74's clock output signal.

Example :_test:SGEN:PDAT:CLOC:VOLT:HIGH?
 might return:
 1.2

:CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW <NRf>
 :<Handle>:SGENERAL:PDATa(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW <NRf>
 :<Handle>:SGENERAL:PDATa(*):TERMINal(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW <NRf>

Parameters <NRf> The lower voltage level of the N4872/74's clock output signal.

Example `_test:SGEN:PDAT:CLOC:VOLT:LOW -0.3`

:CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW?

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW?
 :<Handle>:SGENERAL:PDATa(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW?
 :<Handle>:SGENERAL:PDATa(*):TERMINal(*):CLOCK[:SOURCE]:VOLTage[:LEVel][:IMMediate]:LOW?

Return Value Returns the lower voltage level of the N4872/74's clock output signal.

Example `:_test:SGEN:PDAT:CLOC:VOLT:LOW?`
 might return:
 -0.2

:CLOCK[:SOURCE]:PULSE:DELAY:SWEep

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK[:SOURCE]:PULSE:DELAY:SWEep <NRf>
 :<Handle>:SGENERAL:PDATa(*):CLOCK[:SOURCE]:PULSE:DELAY:SWEep <NRf>
 :<Handle>:SGENERAL:PDATa(*):TERMINal(*):CLOCK[:SOURCE]:PULSE:DELAY:SWEep <NRf>

Parameters <NRf> Delay in periods of the N4872/74's clock output signal. The valid range is: 0 ... 1.0.

Example `:_test:SGEN:PDAT:CLOC:PULSE:DEL:SWE 0.9`

:CLOCK[:SOURCE]:PULSE:DELAY:SWEep?

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK[:SOURCE]:PULSE:DELAY:SWEep?
 :<Handle>:SGENERAL:PDATA(*):CLOCK[:SOURCE]:PULSE:DELAY:SWEep?
 :<Handle>:SGENERAL:PDATA(*):TERMINAL(*):CLOCK[:SOURCE]:PULSE:DELAY:SWEep?

Return Value Sweep delay of the N4872/74's clock output signal in periods.

Example :_test:SGEN:PDAT:CLOC:PULS:DEL:SWE?
 might return:
 9.0E-01

:CLOCK:OUTPUT:IMPedance:EXTERNAL

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK:OUTPUT:IMPedance:EXTERNAL <NRf>
 :<Handle>:SGENERAL:PDATA(*):CLOCK:OUTPUT:IMPedance:EXTERNAL <NRf>
 :<Handle>:SGENERAL:PDATA(*):TERMINAL(*):CLOCK:OUTPUT:IMPedance:EXTERNAL <NRf>

Parameters <NRf> The external termination impedance of the N4872/74's clock output. Only 50.0 Ω is supported.

Example :_test:SGEN:PDAT:CLOC:OUTP:IMP:EXT 50

:CLOCK:OUTPUT:IMPedance:EXTERNAL?

Syntax :<Handle>:CGROUP(*):MODULE(*):CONNECTOR(*):CLOCK:OUTPUT:IMPedance:EXTERNAL?
 :<Handle>:SGENERAL:PDATA(*):CLOCK:OUTPUT:IMPedance:EXTERNAL?
 :<Handle>:SGENERAL:PDATA(*):TERMINAL(*):CLOCK:OUTPUT:IMPedance:EXTERNAL?

Return Value Returns the external termination impedance of the N4872/74's clock output.

Example :_test:sgen:pdat:cloc:outp:imp:ext?
 might return:
 5.0+1

:CLOCK:OUTPut:DIMPedance:EXternal

Syntax :<Handle>:CGRoup(*):MODule(*):CONNector(*):CLOCK:OUTPut:DIMPedance:EXTernal <NRf>
 :<Handle>:SGENeral:PDATA(*):CLOCK:OUTPut:DIMPedance:EXTernal <NRf>
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):CLOCK:OUTPut:DIMPedance:EXTernal <NRf>

Parameters <NRf> Sets the impedance between the OUT and OUT_ outputs of the N4872/74's clock output when the differential termination model is selected (see “*CLOCK:OUTPut:TCONfig*” on page 296). Usually 100 Ohms are used for termination.

Example :_test:CGR:MOD2:CONN:CLOC:OUTP:DIMP:EXT 100

:CLOCK:OUTPut:DIMPedance:EXternal?

Syntax :<Handle>:CGRoup(*):MODule(*):CONNector(*):CLOCK:OUTPut:DIMPedance:EXTernal?
 :<Handle>:SGENeral:PDATA(*):CLOCK:OUTPut:DIMPedance:EXTernal?
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):CLOCK:OUTPut:DIMPedance:EXTernal?

Return Value Returns the differential termination resistance on the N4872/74's clock output.

Example :_test:CGR:MOD2:CONN:CLOC:OUTP:DIMP:EXT?

might return:

1.0+2

:CLOCK:OUTPut:TCONfig

Syntax CGRoup(*):MODule(*):CONNector(*):CLOCK:OUTPut:TCONfig <VOLTage | DIFFerential>
 SGENeral:PDATa(*):CLOCK:OUTPut:TCONfig <VOLTage | DIFFerential>
 SGENeral:PDATa(*):TERMinal(*):CLOCK:OUTPut:TCONfig <VOLTage | DIFFerential>

<VOLTage | DIFFerential> Selects the termination model for the N4872/74's clock output:

- VOLTage selects termination via resistor against a termination voltage (this is the reset value).


If VOLTage is selected, the termination resistor and termination voltage can be set with “:CLOCK:OUTPut:IMPedance:EXTernal” on page 294 and “:CLOCK:OUTPut:TVOLTage” on page 297.

- DIFFerential selects termination via a resistor against the complement output.


If DIFFerential is selected, the differential termination resistor can be set with “:CLOCK:OUTPut:DIMPedance:EXTernal” on page 295.

Description It is necessary to specify how the output signal will be terminated. There are two possible termination models available:

- Via a resistor against a termination voltage; the resistor might be high impedance. Optimum signal performance is achieved with 50 Ohm. In the following picture this is shown for single-ended and differential outputs.

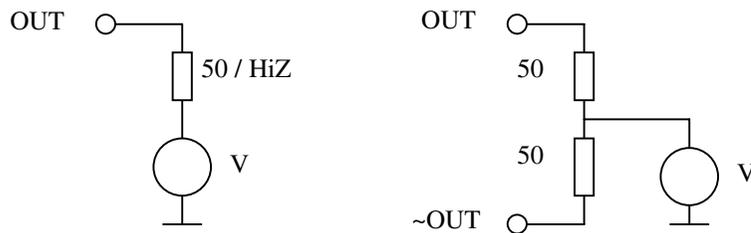

- Via a resistor to the complement output. Optimum signal performance is achieved with 100 Ohms.



Example `:_test:CGR:MOD2:CONN:CLOC:OUTP:TCON VOLT`

:CLOCK:OUTPut:TCONfig?

Syntax `CGRoup(*):MODule(*):CONNector(*)`
`SGENeral:PDATa(*)`
`SGENeral:PDATa(*):TERMinal(*)`

Return Value Returns the termination module for the N4872/74's clock output.

Example `:_test:CGR:MOD2:CONN:CLOC:OUTP:TCON?`
 might return:
 VOLT

:CLOCK:OUTPut:TVOLtage

Syntax `:<Handle>:CGRoup(*):MODule(*):CONNector(*):CLOCK:OUTPut:TVOLtage`
`<NRf>`
`:<Handle>:SGENeral:PDATa(*):CLOCK:OUTPut:TVOLtage <NRf>`
`:<Handle>:SGENeral:PDATa(*):TERMinal(*):CLOCK:OUTPut:TVOLtage <NRf>`

Parameters **<NRf>** Sets the external termination voltage of the N4872/74's clock output, default is 0 volts (ground). Valid range is -2.0 to +3.0 volts.

Example `:_test:CGR:MOD2:CONN:CLOC:OUTP:TVOL 1.0`

:CLOCK:OUTPut:TVOLtage?

Syntax :<Handle>:CGRoup(*):MODule(*):CONNector(*):CLOCK:OUTPut:TVOLtage?
 :<Handle>:SGENeral:PDATA(*):CLOCK:OUTPut:TVOLtage?
 :<Handle>:SGENeral:PDATA(*):TERMinal(*):CLOCK:OUTPut:TVOLtage?

Return Value Returns the current termination voltage of the N4872/74's clock output.

Example :_test:CGR:MOD2:CONN:CLOC:OUTP:TVOL?
 might return:
 3.0E+0

Auxiliary Out Commands

The Auxiliary Out command controls the output at the AUX out of an N4873A/75A module.

:AOUT[:MONitor]

Syntax CGRoup(*):MODule(*):CONNector(*):AOUT[:MONitor] <DME | CLOC>
 SGENeral:PDATA(*):AOUT[:MONitor] <DME | CLOC>
 SGENeral:PDATA(*):TERMinal(*):AOUT[:MONitor] <DME | CLOC>

Parameters <DME | CLOC> Defines the signal at the AUX output of a N4873A/75A module. DMEasurement selects the data stream and CLOCk selects the (recovered) clock.

Example :_test:sgen:pdat:aout DME

:AOUT[:MONitor]?

Syntax CGRoup(*):MODule(*):CONNector(*):AOUT[:MONitor]?
SGENeral:PDATa(*):AOUT[:MONitor]?
SGENeral:PDATa(*):TERMinal(*):AOUT[:MONitor]?

Return Value Returns the signal that at the AUX output of a N4873A/75A module.
Can be DMEasurement (data stream) or CLOCK ((recovered) clock).

Example :_test:sgen:pdatt:aout?
might return:
DME

Port Administration Commands

The following commands are available for managing pulse and data ports. The parameters can be specified separately for pulse and data ports.

The MUX commands—also available for pulse and data ports—are described in *“Timing Parameter Commands” on page 184*.

:APPend

Syntax :<Handle>:SGENeral:PDATa(*):APPend <“Port Type”> [, <No. of Terminals>]
 [, <“Port Name”>], [<Species>]
 :<Handle>:SGENeral:PPULse(*):APPend <“Port Type”> [, <No. of Terminals>]
 [, <“Port Name”>], [<Species>]

Parameters <“Port Type”> A quoted string of the port type, either INPUT_PORT or OUTPUT_PORT, seen from DUT point of view.

[<No. of Terminals>] The integer number of terminals used in the new port (<NR1>). This is an optional parameter.

[<“Port Name”>] A quoted string of the name used to identify the port. This is an optional parameter.

[<Species>] (Optional) Species of the port. Possible values are electrical (ELEC) or optical (OPT). All terminals of the port are assigned this species. Default is electrical.

Creates and appends a new port to the list of ports. The port type is required. The number of terminals, the port name, and species are optional. The suffix of PDATa and PPULse is ignored.

Example :_test:SGEN:PDAT:APP "INPUT_PORT", 4, "DataBus", ELEC
 :_test:SGEN:PPUL:APP "INPUT_PORT", 4, "DataBus", ELEC

:LIST?

Syntax :<Handle>:SGENeral:PDATa(*)LIST?
:<Handle>:SGENeral:PPULse(*)LIST?

Return Value Returns a comma-separated list of port names. If a port has no name specified, an empty quoted string will be returned. The suffix of PDATa or PPULse is ignored.

Example :_test:sgen:pdal:list?
:_test:sgen:ppul:list?
might return:
"DataBus", "AddressBus", "", "ControlBus"

:ATYPes?

Syntax :<Handle>:SGENeral:PDATa(*)ATYPes?
:<Handle>:SGENeral:PPULse(*)ATYPes?

Return Value Returns a comma-separated list of available predefined port TYPES. The suffix of PDATa or PPULse is ignored. Currently there are two types available, INPUT_PORT and OUTPUT_PORT (only for data ports).

Example :_test:sgeneral:pdata:atypes?
might return:
"INPUT_PORT", "OUTPUT_PORT"

:DELeTe

Syntax :<Handle>:SGENeral:PDATa(*)DELeTe
:<Handle>:SGENeral:PPULse(*)DELeTe

Description Deletes the port specified by the suffix of PDATa or PPULse.

Example :_test:SGEN:PDAT1:DEL
:_test:SGEN:PPUL1:DEL

:REName

Syntax :<Handle>:SGENeral:PDATa(*):REName <"New Name">
 :<Handle>:SGENeral:PPULse(*):REName <"New Name">

Parameters <"New Name"> A quoted string of the new name of the port
 Renames the port specified by the suffix of PDATa or PPULse.

Example :_test:sgen:pdat1:ren "AddrBus"
 :_test:sgen:pdat:list?
 "AddrBus"
 :_test:sgen:ppul1:ren "AddrBus"
 :_test:sgen:ppul:list?
 "AddrBus"

:NAME?

Syntax :<Handle>:SGENeral:PDATa(*):NAME?
 :<Handle>:SGENeral:PPULse(*):NAME?

Return Value Returns the name of the specified port.

Example :_test:SGEN:PDAT1:NAME?
 :_test:SGEN:PPUL1:NAME?
 might return:
 "AddrBus"

:NUMBer?

Syntax :<Handle>:SGENeral:PDATa(*):NUMBer?
 :<Handle>:SGENeral:PPULse(*):NUMBer?

Return Value Returns the number of the specified port.

Example :_test:SGEN:PDAT1:NUMB?
 :_test:SGEN:PPUL1:NUMB?
 might return:
 1

:TYPE?

Syntax :<Handle>:SGENeral:PDATa(*):TYPE?
 :<Handle>:SGENeral:PPULse(*):TYPE?

Return Value Returns the TYPE of this port.

Example :_test:SGEN:PDAT1:TYPE?

might return:

"INPUT_PORT"

:_test:SGEN:PPUL1:TYPE?

might return:

"INPUT_PORT"

:CALibration:CDElay

Syntax :<Handle>:SGENeral:PDATa(*):CALibration:CDElay <Cable Delay>
 :<Handle>:SGENeral:PPULse(*):CALibration:CDElay <Cable Delay>

Parameters <Cable Delay> Cable Delay value (<NRF>).

Sets a cable delay for the specified port to synchronize the signals at the DUT terminals.

NOTE Delay Auto Calibration must be performed before the cable delay can be set. See “:<Handle>:SGENeral:GLOBal:CALibration:SELF DELay” on page 143.

Example :_test:SGEN:PDAT1:CAL:CDEL 6.5e-9

:CALibration:CDElay?

Syntax :<Handle>:SGENeral:PDATa(*):CALibration:CDElay?
 :<Handle>:SGENeral:PPULse(*):CALibration:CDElay?

Return Value Returns the current cable delay for the specified port.

Example :_test:SGEN:PDAT1:CAL:CDEL?

:_test:SGEN:PPUL1:CAL:CDEL?

might return:

6.500000E-009

:SPECies?

- Syntax** :<Handle>:SGENeral:PDATa(*):SPECies?
 :<Handle>:SGENeral:PPULse(*):SPECies?
- Return Value** Returns the port's species. This can be either electrical (ELEC) or optical (OPT).
- Example** :_test:SGEN:PDAT1:SPEC?
 :_test:SGEN:PPUL1:SPEC?
 might return:
 ELEC

Terminal Administration Commands

The following commands are available for administration of terminals. The parameters can be specified separately for pulse and data ports.

:APPend

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):APPend [<"Terminal Name">]
[,<Position>]
:<Handle>:SGENeral:PPULse(*):TERMinal(*):APPend [<"Terminal Name">]
[,<Position>]

Parameters [<"Terminal Name">] Quoted String of the name of new terminal.

[<Position>] Integer number of the position where the new terminal will be added.

Creates and appends a new terminal to a port. The terminal name and the position of the new terminal are optional. If the specified position is zero, the new terminal is placed at the beginning of the list. If "Position" is omitted or greater than the number of terminals, the new terminal is appended to the list. Otherwise, the new terminal is inserted *after* the specified position.

Example :_test:SGEN:PDAT1:TERM1:APP "Data5", 5
:_test:SGEN:PPUL1:TERM1:APP "Clock", 5

:LIST?

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):LIST?
:<Handle>:SGENeral:PPULse(*):TERMinal(*):LIST?

Return Value Returns a comma-separated list of all terminal names contained in the specified port.

Example :_test:SGEN:PDAT1:TERM1:LIST?
"T1", "T2", "T3", "T4", "Data5"
:_test:SGEN:PPUL1:TERM1:LIST?
"T1", "T2", "T3", "T4", "Clock"

:DElete

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):DElete
:<Handle>:SGENeral:PPULse(*):TERMinal(*):DElete

Description Deletes the specified terminal.

Example :_test:SGEN:PDAT1:TERM1:DEL
:_test:SGEN:PPUL1:TERM1:DEL

:FETch:SStatus?

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):FETch:SStatus?

Return Value Returns the status of the specified terminal:

SYNCing Indicates that the terminal is syncing.

SUCceeded Indicates that synchronization was successful.

FAILed Indicates that the synchronization failed.

NAVailable Indicates that the terminal is not available.

STOP Indicates that the system is not running.

Example :_test:SGEN:PDAT1:TERM1:FET:SST
might return:
SYNC, SUCC, STOP

:REName

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):REName <“New Name”>
:<Handle>:SGENeral:PPULse(*):TERMinal(*):REName <“New Name”>

Parameters <“New Name”> A quoted string of the new name for the terminal.
Renames the specified terminal.

Example :_test:sgen:pdatt1:term5:REN "Addr5"
 :_test:SGEN:PDAT1:TERM1:LIST?

 :_test:sgen:ppul1:term5:REN "Addr5"
 :_test:SGEN:PPUL1:TERM1:LIST?

might return:

"T1", "T2", "T3", "T4", "Addr5"

:NAME?

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):NAME?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):NAME?

Return Value Returns the name of the specified terminal.

Example :_test:SGEN:PDAT1:TERM1:NAME?
 :_test:SGEN:PPUL1:TERM1:NAME?

might return:

"T1"

:TYPE?

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):TYPE?
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):TYPE?

Return Value Returns the type of the specified terminal.

Example :_test:SGEN:PDAT1:TERM1:TYPE?

might return:

"E4843A"

:MOVE

Syntax :<Handle>:SGENeral:PDATa(*):TERMinal(*):MOVE <Distance>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):MOVE <Distance>

Parameters <Distance> Number of positions this terminal is to be moved by (<NR1>).

Moves the specified terminal to a new position.

Example `:_test:SGEN:PDAT1:TERM1:MOVE 1`
 `:_test:SGEN:PDAT1:TERM1:LIST?`

might return:

`"T2", "T1", "T3", "T4", "Addr5"`

`:_test:SGEN:PPUL1:TERM1:MOVE 1`
`:_test:SGEN:PPUL1:TERM1:LIST?`

might return:

`"T2", "T1", "T3", "T4", "Addr5"`

:CALibration:CDElay

Syntax `<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration:CDElay <Cable Delay>`

`<Handle>:SGENeral:PPULse(*):TERMinal(*):CALibration:CDElay`
`<Cable Delay>`

Sets a cable delay for the specified terminal in the specific port to synchronize the signals at the DUT terminals.

NOTE Delay Auto Calibration must be performed before the cable delay can be set. See “*:<Handle>:SGENeral:GLOBal:CALibration:SELF DELay*” on page 143.

Parameters `<Cable Delay>` Cable Delay value (<NRf>).

Example `:_test:SGEN:PDAT1:TERM1:CAL:CDEL 6.5e-9`
 `:_test:SGEN:PPUL1:TERM1:CAL:CDEL 6.5e-9`

:CALibration:CDElay?

Syntax `<Handle>:SGENeral:PDATa(*):TERMinal(*):CALibration:CDElay?`

`<Handle>:SGENeral:PPULse(*):TERMinal(*):CALibration:CDElay?`

Return Value Returns the current cable delay for the specified terminal of the specified terminal.

Example `:_test:SGEN:PDAT1:TERM1:CAL:CDEL?`
 `:_test:SGEN:PPUL1:TERM1:CAL:CDEL?`
 might return:
 `6.500000E-009`

Connector Administration Commands

The following commands are available to associate the connectors of the Agilent 81250 System to the terminals of the DUT. Other connector administration commands can be found in the “[:CGROUP(*):MODULE(*):CONNECTOR(*) Subsystem” on page 129.

The commands are available for pulse and data ports. They build the :<Handle>:SGENERAL:CONNECT subsystem.

:REMove

Syntax :<Handle>:SGENERAL:CONNECT:PDATa(*):REMove
:<Handle>:SGENERAL:CONNECT:PDATa(*):TERMinal(*):REMove
:<Handle>:SGENERAL:CONNECT:PPULse(*):REMove
:<Handle>:SGENERAL:CONNECT:PPULse(*):TERMinal(*):REMove

Description Disconnects all terminals within the specified port, or the specified terminal.

Example :_test:sgen:conn:pdat2:rem
:_test:sgeneral:connect:pdata1:terminal2:remove
:_test:sgen:conn:ppul2:rem
:_test:sgeneral:connect:ppull1:terminal2:remove

:TERMI n al(*):[TO]

Syntax :<Handle>:SGENeral:CONNect:PDATa(*):TERMI n al(*):[TO] <@ChannelList>
 :<Handle>:SGENeral:CONNect:PPULse(*):TERMI n al(*):[TO] <@ChannelList>

Parameters <@ChannelList> List of channels.

Connects the specified terminal to the specified channel or channels. If the number of connectors exceeds the number of terminals defined in the specified port, the connection will be continued to the next port. In other words, the suffix of the port and the suffix of the terminal are used as a start value. Only connectors of the same type can be combined to a port.

The syntax of the channel list is as follows:

```

<ChannelListExpr> ::= “(@”<ChannelList>“)”
<ChannelList>    ::= <ChannelListElem> [“,” <ChannelListElem>]
<ChannelListElem> ::= <Connector> | (<Connector> “.” <Connector>)
<Connector>     ::= <ClockGroupNr><ModuleNr><ConnectorNr>
<ClockGroupNr>  ::= <Digit><Digit>
<ModuleNr>      ::= <Digit><Digit>
<ConnectorNr>   ::= <Digit><Digit><Digit>
<Digit>         ::= “0” | “1” | “2” | “3” | “4” | “5” | “6” | “7” | “8” |
                    “9”
  
```

Syntax Examples:

- (@0102004) specifies connector 4 in clock group 1, module 2
- (@0102001:0102004,0103001) specifies connectors 1 to 4 of module 2 and connector 1 of module 3, both in clockgroup 1

Example :_test:SGEN:CONN:PDAT1:TERM2:TO (@0102001)
 :_test:SGEN:CONN:PPUL1:TERM2:TO (@0102001)

:TERMinal(*):[TO]?

Syntax :<Handle>:SGENeral:CONNect:PDATa(*):TERMinal(*):[TO]? [ALL]
:<Handle>:SGENeral:CONNect:PPULse(*):TERMinal(*):[TO]? [ALL]

Parameters **ALL** If specified, returns all channels connected to this terminal (only when channel addition is used).

This query returns the channel to which the specified terminal is connected. If the terminal is not connected an empty channel list is returned (for example, @). The optional parameter ALL returns a more detailed list of connectors if the channel add mode is active.

Example :_test:sgen:conn:pdat1:term2:to? all
:_test:sgen:conn:ppull1:term2:to? all

might return:

(@0102001, 0102002)

Error Analysis Commands

The Error Analysis Commands are used to report and reset bit errors on specific ports or terminals.

:FETCh:ERRor:ANY?

Syntax :<Handle>:SGENeral:PDATa(*):FETCh:ERRor:ANY?
:<Handle>:SGENeral:PDATa(*):TERMinal(*):FETCh:ERRor:ANY?

Return Value Returns 0 for no errors, 1 if an error was found for the specified data port or terminal.

This can be used to increase program speed. Uploading of memory segments can be completely avoided, when it is known, that there are no errors at all.

Example :_test:SGEN:PDAT1:FETC:ERR:ANY?
:_test:SGEN:PDAT1:TERM2:FETC:ERR:ANY?
might return:
0

:FETCh[:ECOunt]?

Syntax :<Handle>:SGENeral:PDATa(*):FETCh[:ECOunt]? [(<TermChannelList >) | <PSUM>]

Parameters <PSUM> Generates an accumulation of the received bits count (Accumulated Number of Bits) and the error bits count (Accumulated Number of Errors) for all terminals of the whole port.

<TermChannelList> Selects specific terminals of a data port. If the argument is omitted, all measured values within the specified port are reported.

In the error count mode this query returns the number of received bits and the number of erroneous bits. The counters are set to zero after a stop/start request or reset. The results are contained in a comma-separated list.

For example, the channel list (@1:3) addresses 3 channels within a data port and reports 6 values in a comma-separated list, for example, 2.345e5,0,2.33e5,0,2.32e5,5. Each pair of values relates to one terminal. The first value is the number of received bits, the second value is the number of erroneous bits (failed bits). One pair is sampled at the same time, the subsequent pair is sampled some cycles later. In the example, there are 5 errors counted at terminal 3.

The syntax of the terminal channel list is as follows:

```

<TermChannelListExpr ::= “(@”<TermChannelList>“)”
>
<TermChannelList> ::= <TermChannelListElem> [“,”
<TermChannelListElem>]
<TermChannelListElem ::= <TermNr> | (<TermNr> “:” <TermNr>)
>
<TermNr> ::= <Digit>[<Digit>]
<Digit> ::= “0” | “1” | “2” | “3” | “4” | “5” | “6” | “7”
| “8” | “9”

```

Return Value **On parameter <PSUM>:**

Comma-separated list of two exponential float values.

- The first value represents the accumulation of the received bits count (Accumulated Number of Bits).
- The second value is the accumulation of the the error bits count (Accumulated Number of Errors) for all terminals of the whole port.

On parameter <TermChannelList>:

Comma-separated list of tuple exponential float values. There are as many tuples as addressed by the <TermChannelList>. The values of the tuple are likewise comma-separated.

- The first value of the tuple represents the accumulation of the received bits count (Accumulated Number of Bits).
- The second value of the tuple represents the accumulation of the error bits count (Accumulated Number of Errors) for all terminals of the whole port.

When no parameter provided:

Comma-separated list of tuple exponential float values. There are as many tuples as terminals contained in the specified port. The values of the tuple are likewise comma-separated.

- The first value of the tuple represents the accumulation of the received bits count (Accumulated Number of Bits).

- The second value of the tuple is the accumulation of the the error bits count (Accumulated Number of Errors) for all terminals of the whole port.

Syntax Examples: (@4) specifies terminal 4.

(@3:5,9) specifies terminals 3, 4, 5 and 9.

Example :_test:SGEN:PDAT1:FETC? PSUM

might return:

5.1967356791200e+012, 4.1612064440000e+009

:_test:SGEN:PDAT1:FETC? (@1:3)

might return:

3.2480134390400e+011, 1.4717679000000e+008,

3.2458887171200e+011, 1.6075325500000e+008,

3.2459149132800e+011, 1.7538254400000e+008

:_test:SGEN:PDAT1:FETC?

might return:

3.2480134390400e+011, 1.4717679000000e+008,

3.2458887171200e+011, 1.6075325500000e+008,

3.2459149132800e+011, 1.7538254400000e+008,

3.2502299556800e+011, 1.9273679100000e+008

NOTE If you have a finite sequence and are interested in the final result, you should query the system state before trying to fetch the error rate results. With the command :sgen:glob:syst:stat? you can check when the system has FINished the sequence generation. Then stop the system by :sgen:glob:init:cont OFF. Now it is save to fetch the error rate results.

If you have an infinite sequence or want intermediate results anyway, you can query the error results an any time. You always get the number of received bits and the number or erroneous bits. If you query soon after start, it can happen that the number of received bits is 0. Then, of course, the number of errors is also 0. Ignore these results and query again.

:ECOUNT:RESet

Syntax :<Handle>:SGENeral:PDATa(*):ECOUNT:RESet[(<ChannelList>)]

Description This command resets the “received bit counter” and the “failed bit counter” to zero. If the argument is omitted all connected terminals within a port are reset to zero. The channel list specifies a list of terminals e.g. (@1:3,5) addresses the terminals 1,2,3,5 and these counters are set to 0.

Example :_test:SGEN:PDAT1:ECO:RES (@1:3,5)

Clock Mode Commands

NOTE The clock mode command is only valid for the E4862B data generator frontends.

The clock mode command is used to specify whether pulse (normal) or clock (high performance) mode is used. In clock mode, a precision clock signal is generated, with 50 % duty cycle and very low jitter (given by the clock module – the E4808A clock module should be used).

:SIGNal:MODE

This command sets the mode of the clock signal of E4862B data generator frontends. The performance mode can be either **CLOCK** (high-performance) or **PULSE** (normal).

NOTE Executing this command while the system is running causes the system to be restarted.

Syntax :<HANDLE>[:**CGROUP***]:**MODUle***:**CONNector***:**DIGital**:**STIMulus**:**SIGNal**:
MODE PULSE | **CLOCK**
 :<HANDLE>:**SGENeral**:**PDATa***:**DIGital**:**STIMulus**:**SIGNal**:**MODE**
PULSE | **CLOCK**
 :<HANDLE>:**SGENeral**:**PDATa***:**TERMI**nal*:**DIGital**:**STIMulus**:**SIGNal**:**MODE**
PULSE | **CLOCK**
 :<HANDLE>:**SGENeral**:**PPULse***:**DIGital**:**STIMulus**:**SIGNal**:**MODE**
PULSE | **CLOCK**
 :<HANDLE>:**SGENeral**:**PPULse***:**TERMI**nal*:**DIGital**:**STIMulus**:**SIGNal**:**MODE**
PULSE | **CLOCK**

Parameters **PULSE** Pulse mode (normal) is used.

CLOCK Clock mode (high performance) is used.

Example :_test:SGEN:PDAT1:DIG:SIGN:STIM:MODE CLOC
 :_test:SGEN:PDAT1:TERM1:DIG:STIM:SIGN:MODE CLOCK
 :_test:SGEN:PPUL1:DIG:SIGN:MODE CLOC
 :_test:SGEN:PPUL1:TERM1:DIG:STIM:SIGN:MODE CLOCK
 :_test:CGROUP1:MODUle2:CONNector4:DIGital:SIGNal:MODE CLOCK

:SIGNal:MODE?

Syntax :<HANDLE>[:CGRoup*]:MODule*:CONNector*:DIGital:STIMulus:SIGNal:MODE?
 :<HANDLE>:SGENeral:PDATa*:DIGital:STIMulus:SIGNal:MODE?
 :<HANDLE>:SGENeral:PDATa*:TERMinal*:DIGital:STIMulus:SIGNal:MODE?
 :<HANDLE>:SGENeral:PPULse*:DIGital:STIMulus:SIGNal:MODE?
 :<HANDLE>:SGENeral:PPULse*:TERMinal*:DIGital:STIMulus:SIGNal:MODE?

Return Value Returns the mode for the clock signal of E4862B data generator frontends: either CLOck or PULSe.

- PULSe
Pulse mode (normal) is used.
- CLOck
Clock mode (high performance) is used.

Example :_test:SGEN:PDAT1:DIG:SIGN:STIM:MODE?
 :_test:SGEN:PDAT1:TERM1:DIG:STIM:SIGN:MODE?
 :_test:SGEN:PPUL1:DIG:SIGN:MODE?
 :_test:SGEN:PPUL1:TERM1:DIG:STIM:SIGN:MODE?
 :_test:CGRoup1:MODule2:CONNector4:DIGital:SIGNal:MODE?

might return:

CLOC

Format Parameter Commands

The commands for specifying the format parameters are available on port, terminal and connector level. The parameters can be specified separately for pulse and data ports.

:FORMat

Syntax :<Handle>:SGENeral:PDATa(*):DIGital[:STIMulus]:SIGNal:FORMat <RZ | NRZ | R1>
 :<Handle>:SGENeral:PDATa(*):TERMinal(*):DIGital[:STIMulus]:SIGNal:FORMat <RZ | NRZ | R1>
 :<Handle>:SGENeral:PPULse(*):DIGital[:STIMulus]:SIGNal:FORMat <RZ | NRZ | R1>
 :<Handle>:SGENeral:PPULse(*):TERMinal(*):DIGital[:STIMulus]:SIGNal:FORMat <RZ | NRZ | R1>
 :<Handle>[:CGRoup(*):MODULE(*):CONNector(*):DIGital[:STIMulus]:SIGNal:FORMat <RZ | NRZ | R1>

Parameters <RZ | NRZ | R1> Sets the output connector data format to either RZ, NRZ or R1.

The format of the data out stream can be specified here. Setting the Format to RZ or R1 may generate an error that the “WIDTH” is out of range. The E4862A and E4864A frontends and N4872A and N4874A modules support only NRZ.

Example :_test:SGEN:PDAT1:DIG:SIGN:FORM RZ
 :_test:SGEN:PDAT1:TERM1:DIG:STIM:SIGN:FORM RZ
 :_test:SGEN:PPUL1:DIG:SIGN:FORM RZ
 :_test:SGEN:PPUL1:TERM1:DIG:STIM:SIGN:FORM RZ
 :_test:CGROUP1:MODULE2:CONNECTOR4:DIGITAL:SIGNAL:FORMAT RZ

:FORMat?


Syntax :<Handle>:SGENeral:**PDATa**(*):DIGital[:STIMulus]:SIGNal:FORMat?
 :<Handle>:SGENeral:**PDATa**(*):**TERMinal**(*):DIGital[:STIMulus]:SIGNal
 :FORMat?
 :<Handle>:SGENeral:**PPULse**(*):DIGital[:STIMulus]:SIGNal:FORMat?
 :<Handle>:SGENeral:**PPULse**(*):**TERMinal**(*):DIGital[:STIMulus]:SIGNal
 :FORMat?
 :<Handle>[:CGRoup(*)]:MODule(*):**CONNector**(*):DIGital[:STIMulus]:SIGNal
 :FORMat?

Return Value Returns the current data format state.

Example :_test:SGEN:PDAT1:DIG:SIGN:FORM?
 :_test:SGEN:PDAT1:TERM1:DIG:STIM:SIGN:format?
 :_test:SGEN:PPUL1:DIG:SIGN:FORM?
 :_test:SGEN:PPUL1:TERM1:DIG:STIM:SIGN:format?
 :_test:CGROUP1:MODULE2:CONNECTOR4:DIGITAL:SIGNAL:FORMAT?

might return:

RZ



Segment Import and Export Language

The Segment Import and Export Tool enables the Agilent 81250 System to import and export connector trace data from/to an ASCII source file.

The syntax of the segment import and export tool enables you to create data segments in any text editor.

You can also export segments that have been set up in the graphical user interface to ASCII files and modify these files as required.

The following details are described:

- *“The Language Syntax” on page 322*
- *“Concepts” on page 326*
- *“Default Settings” on page 333*
- *“Examples” on page 333*


The Language Syntax

Syntax flow diagrams (also known as railroad diagrams) are used to provide pictorial representations of syntax.

Vector Variable Construct

The vector import language is contained in an ASCII text file and contains one or more **Vector Variable constructs**. A Vector Variable construct is the highest level construct that may be specified and is itself built from lower level constructs.


The format of the **Vector Variable construct** is shown below:

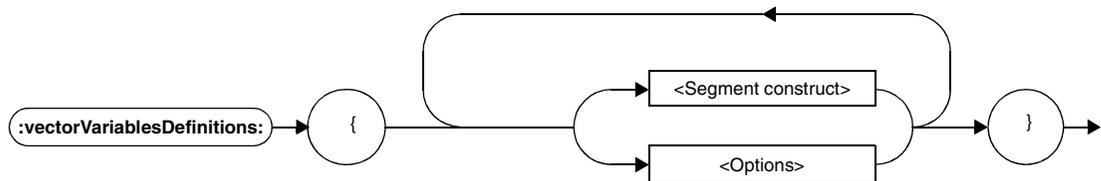

<Options> contains 1 or more default parameters that may be overridden as necessary. There are two scopes for options, **vector variable scope and pattern scope**. The options constructs will be described in more detail in *“Options” on page 323*.

Segment Construct

The **Segment construct** contains **segment** information. A segment is a unit of information acceptable to the Agilent 81250 System and may contain either connector trace data or parameters necessary for the operation of the instrument. The following syntax diagram shows the composition of a segment construct:

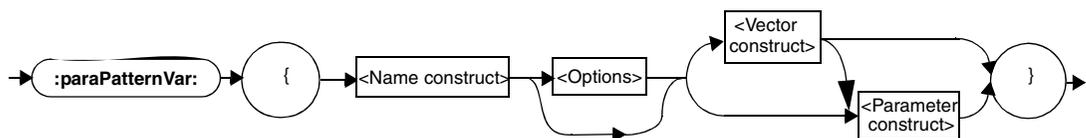

Name Construct


The **Name construct** specifies a name for the segment:



where <SEG_NAME> is an ASCII string representing the segment name. The segment name *must* begin with a letter, which may be followed by an alphanumeric string. Underscores are allowed, whitespaces are not.

Options

The **Options** syntax is defined in the following diagram:

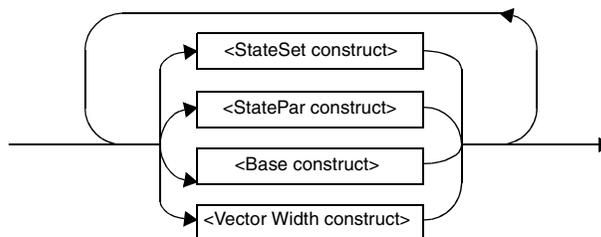


Options defined within a vector variable scope remain valid for the duration of the vector variable construct. However, options may also be specified within a segment construct in which case they are valid only for the duration of the segment construct. As soon as the segment construct goes out of scope the options valid at the vector variable scope re-apply (see “*Scopes*” on page 328 for a more detailed definition of scopes).

StatePar Construct

The **StatePar** construct allows specification of one or more **state sets**. A state set is the specification of waveform characters that may legally be used within the **:vectors:** statement.

A state set consists of a state set name and its corresponding coding. The state set name is referred to by the StatePar construct:

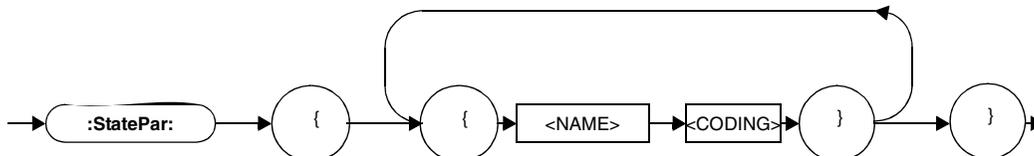

where **<NAME>** is an ASCII string representing the name of the coding, and **<CODING>** is an ASCII string representing the coding. Two state sets are supplied as default: **{D "01"}** and **{R "0 x1"}**, see *"Coding" on page 326*

StateSet Construct

The **StateSet** construct selects a coding previously defined by the StatePar command. The name supplied as an argument indicates which coding should be used:



where **<NAME>** is an ASCII string representing the name of the coding. The default state set is **D**.

Base Construct

The **Base** construct selects the nature of the strings representing the input vectors. There are three possibilities: **hex (h)**, **decimal (d)** or **waveform (w)**.




<BASE> is one of **w**, **h**, or **d**. The default base is **w**.

Vector Width Construct

The **Vector width construct** allows the specification of the width in states of each vector. Should the number of states supplied be less than that specified in the **:vectorWidth:** command, then the vector is padded out on its left side using the left most supplied state. Should the supplied vector be too long then it is clipped on the left side until it contains exactly the necessary number of states.


If no vector width statement is present, then the length of the first supplied vector is used as the width for all subsequent vectors:



where <INTEGER> is an integer value between 1 and 1024.

Vector Construct


The **Vector construct** specifies the content of connector trace data:

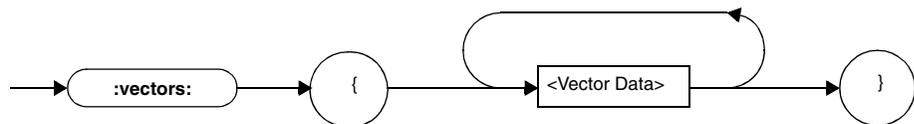

<Vector Data> is one or more strings of hex, decimal or waveform characters. Each string is delimited by a new line. The waveform characters are specified by the currently active state set. The vector format (i.e. hex, decimal or waveform) is specified by the **:base:** command described in “*Base Construct*” on page 324.

Parameter Construct

The counterpart to the vector construct is the **Parameter construct**. This construct enables the input of supplementary segment information:

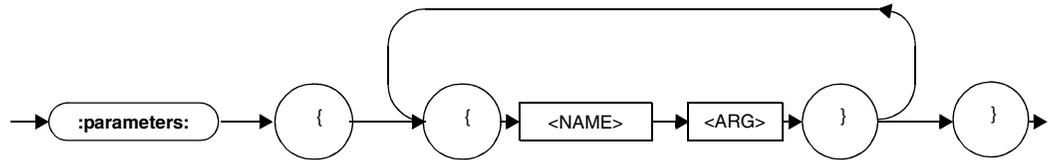

where <NAME> is an ASCII string representing the name of the argument and <ARG> is the argument type. Each argument pair is enclosed within brackets. The range of possible parameters is described more fully in the section “*Parameter Segments*” on page 331 below.

Concepts

This section describes some of the more important concepts of the vector import language.

Coding

In this section, the coding mechanism is described in more detail.

The goal of the Vector Import tool is to be able to load one or more sequences of binary data to the Agilent 81250 System. The binary data contains waveforms to be presented to the connectors of a hardware device. However, the use of pure binary is difficult for humans to interpret and therefore for programming purposes an alternative representation is necessary.

Firstly, we demonstrate the decoding of a vector that is in waveform characters.

Using Base w

Consider the following portion of import language code:

```
:statePar: { {B "0 x1")    #define state set B to have coding "0 x1"
:stateSet: B              #select State set B
:base: w                  #use waveform characters
:vectorWidth: 5          #vector is 5 states wide
:vectors:
{
  001xx                  #this is the vector
}
```

Let us examine the *:statePar:* statement. A state set name B is associated with the coding “0 x1”. The order of the characters “0 x1” is particularly important as it implies the underlying binary values. Starting with 0, the coding assumes increasing order from left to right.

Each of the waveform characters represents a state. To represent three waveform characters, two bits are required. With two bits there are 4 binary values available. The value 01 must be represented by ‘blank’ because this is not a valid waveform character. Therefore, the binary values of the states are: 0 = 00, ‘blank’= 01, x = 10 and 1 = 11. Enough information is now available to decode the vector: 001xx = 00 00 11 10 10

Coding	Memory Representation	Hardware Representation
0	00	0
'blank'	n/a	n/a
x	10	Don't care
1	11	1

Coding	Memory Representation	Hardware Representation
0	0	0
1	1	1

Here is the same example using a hexadecimal base and the coding “0 x1”:

Using Base h (hexadecimal)

```
:statePar: { { B "0 x1"} #define state set B to have coding "0 x1"
:stateSet: B           #select state set B
:base: h               #use hex characters
:vectorWidth: 5       #vector is 5 states wide
:vectors:
{
  03a                  #this is the vector
}
```

Each hexadecimal character needs 4 bits and so in the above example the vector is 12 bits wide. As only 10 bits are necessary to represent 5 vectors, the leftmost 2 bits are ignored:

0000 0011 1010

Finally, the same example using base d (decimal):

Using Base d

```
:statePar: { { B "0 x1"} #define state set B to have coding "0 x1"
:stateSet: B           #select state set B
:base: d               #use decimal characters
:vectorWidth: 5       #vector is 5 states wide
:vectors:
{
  58                   #this is the vector
}
```

The decimal value 58 is decoded as a 32 bit unsigned integer:

00000000 00000000 00000000 **00111010**

the 10 rightmost bits being the vector.

When using hexadecimal and decimal bases, decoding still requires a valid state set to know the bit width of each state.

Scopes

Scopes are important to the lifetime of optional variables. There are 2 scopes, vector variable scope and parameter scope. In the following diagram, the `:base:` parameter is used to illustrate scope. At the start of the program fragment, base w is defined (although base w is default we define it for demonstration purposes). The first grey shaded area shows the scope of the base w command. Waveform characters are thus used in SegA. In SegB a new base h is specified. The white box shows the scope of the base h command.

As the base h command was defined with parameter scope, as soon as the definition for SegB ends, so does the scope of the base h command. The base reverts to that of the previously defined base w.

Then, still within vector variable scope, base d is defined. This remains the base until the end of the vector variables definition.

```

:vectorVariablesDefinitions:          #start of vector variable scope
{
  :base: w
  :paraPatternVar:
  {
    :name: SegA
    :vectors:
    {
      1101110110101
    }
  }
  :paraPatternVar:
  {
    :name: SegB
    :base: h                          # start of pattern scope
    :vectors:                          # base h is valid
    {                                   #
      f7df                              #
    }                                   #
  }                                     #
                                        # until here
# vector variable scope
# base w is valid

  :base: d                            # base d supersedes base w
  :paraPatternVar:
  {
    :name: SegC
    :vectors:
    {
      243
    }
  }
}
# end of vector variable scope

```

Vector Padding and Clipping

The vector import tool ensures that all vectors input from the source file have the correct length. All following padding and clipping examples are shown in base w; i.e. waveform characters. Padding and clipping in hex or decimal bases behave as though the representation were first converted to waveform characters.


Padding

A vector that is shorter than necessary must be padded to the correct length. For example if a vector width of 10 states is being used, the Vector Import Tool would expand 01x to 000000001x. The Import Tool knowing that 7 states were missing, takes the leftmost state, in this case '0' and fills out the vector on the left side until it is of the correct length. Padding can be useful when the same vector cluster is repeated many times. Consider the following example:

```
Without Padding :statePar: { {B "0 x1"} } #define state set B to have coding "0 x1"
:stateSet: B           #select state set B
:base: w               #use waveform characters
:vectorWidth: 8       #vector is 8 states wide
:vectors
{
xxxxxxxx
}
```

It would be possible to rewrite this code snippet thus:

```
With Padding :statePar: { {B "0 x1"} } #define state set B to have coding
"0 x1"
:stateSet: B           #select state set B
:base: w               #use waveform characters
:vectorWidth: 8       #vector is 8 states wide
:vectors
{
x
}
```

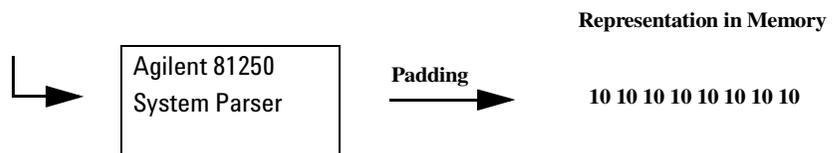

The Vector Import Tool recognizes that 7 states are missing, and uses the left-most (and only) state to pad out the vector. A reduction in disk storage is possible in vector files with a high degree of repetition.

Clipping

A supplied vector that is too long will be clipped on its left side until it is of the correct length. For example, using a vector width of 10, `xxxx000000001x` would be clipped to `000000001x`.

Parameter Segments

Parameter segments allow the input of parameter variables into the Agilent 81250 System. The data part of a parameter segment consists of a string. The string consists of one or more name-parameter pairs enclosed by parentheses. The string and the name-parameter pairs compare to the rules of SCPI expressions.

There are three data segment types.

- Memory segments
- PRBS segments
- PRWS segments
- SFI-5 segments

Predefined Parameter Names

For the three segment types the following predefined parameter names and values are valid:

Predefined Parameter Names	Memory Segments	PRBS Segments	PRWS Segments	SFI-5 Segments
_Type	(MEMORY)	(PRBS)	(PRWS)	(SFI5)
_Rotating	not applicable [n/a]	()	()	()
_Polynom	n/a	("2^5-1")...("2^15-1") ^a	("2^5-1")...("2^15-1") ^a	("2^7-1"), ("2^11-1"), ("2^15-1"), ("2^23-1"), ("2^31-1")
_Logic	n/a	(NORMAL) or (INVERTED)	(NORMAL) or (INVERTED)	(NORMAL) or (INVERTED)
_PRxSType	n/a	(PURE) or (ERRORED) or (DENSITY) or (EXTENDED)	(PURE) or (ERRORED) or (DENSITY) or (EXTENDED)	(PURE)
_FramingBytes	n/a	n/a	n/a	32 bit binary-string enclosed in '()
_ExpansionHeader	n/a	n/a	n/a	32 bit binary-string enclosed in '()
_Errors [when (ERRORED) is selected]	n/a	(0)...(max length of selected PRxS)	(0)...(max length of selected PRxS)	n/a

Predefined Parameter Names	Memory Segments	PRBS Segments	PRWS Segments	SFI-5 Segments
_Density [when (DENSITY) is selected]	n/a	("1/8") or ("1/4") or ("1/2") or ("3/4") or ("7/8")	("1/8") or ("1/4") or ("1/2") or ("3/4") or ("7/8")	n/a
_Which [when (EXTENDED) is selected]	n/a	(ZERO) or (ONE)	(ZERO) or (ONE)	n/a
_Number [when (EXTENDED) is selected]	n/a	(0)...(max length of selected PRxS)	(0)...(max length of selected PRxS)	n/a

^a PRBS and PRWS both also support 2^{23} and 2^{31} . These polynomials must be PURE, because they do not fit into the RAM.

Default Segment for SFI-5

There is a default segment for SFI-5, which has the following settings:

Parameter	Value
_Type	(SFI5)
_Rotating	()
_Polynom	("2 ¹⁵ -1")
_Logic	(NORMAL) or (INVERTED)
_PRxSType	(PURE)
_FramingBytes	("11110110111101100010100000101000")
_ExpansionHeader	("10101010101010101010101010101010")

Default Settings

The Vector Import tool provides default settings for the following parameters:

Parameter	Default Value
:statePar:	{D 01} /R "0 x1"
:stateSet:	D
:base:	w
:vectorWidth:	length of first vector

The default values are valid in both Vector variable and parameter scopes.

Examples

The following portion of vector import code illustrates the use of a parameter segment:

- “*Example: Memory Type Segment*” on page 334 shows a data pattern segment, a memory type segment.
- “*Example: PRBS Type Segment*” on page 334 shows a pure 2^8-1 PRBS with normal output mode, a PRBS segment type.
- “*Example: PRWS Type Segment*” on page 335 shows a $2^{10}-1$ PRWS with 10 errors inserted and with inverted output mode.
- “*Example: SFI5 Type Segment*” on page 335 shows a $2^{15}-1$ SFI-5 segment.

Example: Memory Type Segment

```

:vectorVariablesDefinitions:
{
  :paraPatternVar:
  {
    :name: InitData
    :statePart: { {A 01} }
    :stateSet: A
    :vectorWidth: 4
    :vectors:
    {
      1111
      0000
      1111
      0000
      1111
      0000
      1111
      0000
      1111
      0000
      1111
      0000
    }
    :parameters:           #Predefined parameter names
    {                       #start with '_'
      { _Type (MEMORY) }    #parameter values
    }                       #are always
  }                         #enclosed in '()'
}

```

Example: PRBS Type Segment

```

:vectorVariablesDefinitions:
{
  :paraPatternVar:
  {
    :name: prw
    :parameters:
    {
      { _Type (PRWS) }      #Predefined parameter names
      { _Rotating () }      #start with '_'
      { _PRxSType (ERRORED) } #parameter values
      { _Polynom ("2^10-1") } #are always
      { _Logic (INVERTED) } #enclosed in '()'
    }
  }
}

```

Example: PRWS Type Segment

```
:vectorVariablesDefinitions:
{
  :paraPatternVar:
  {
    :name: payload
    :parameters:
    {
      { _Type (PRBS) }           #Predefined parameter names
      { _Rotating () }         #start with '_'
      { _PRxSType (PURE) }     #parameter values
      { _Polynom ("2^8-1") }   #are always
      { _Logic (NORMAL) }     #enclosed in '()'
    }
  }
}
```

Example: SFI5 Type Segment

```
:vectorVariablesDefinitions:
{
  :paraPatternVar:
  {
    :name: sfi5_example
    :parameters:
    {
      #Predefined parameter names
      #start with '_'
      #parameter values
      #are always
      #enclosed in '()'

      { _Type (SFI5) }
      { _FramingBytes ("11110110111101100010100000101000") }
      { _ExpansionHeader ("10101010101010101010100000000000") }
      { _Rotating () }
      { _PRxSType (PURE) }
      { _Logic (NORMAL) }
      { _Polynom ("2^15-1") }
    }
  }
}
```


Example Code

NOTE Instead of using the SCPI commands, we recommend to use the plug & play programming interface. For an online help on the VXIPNP functions, refer to `hp81200.hlp` provided with the plug & play functions.

The following is an example of how to use plug & play functions to simplify programming:

- *“Main.cpp Application Code Using VXI Plug&Play” on page 338*

The following provide the complete code for the *“Example C++ Program” on page 40*:

- *“Lib.cpp Interface Class Library Code” on page 351*
- *“Main.cpp Application Code” on page 356*

Main.cpp Application Code Using VXI Plug&Play

The following is an example of implementing plug & play functionality. It is recommended that you use the plug & play functionality to program the system.

```
// main.cpp
// This is a small demo program showing how to use
// the remote interface of the 81200A user software

//
// It demonstrates how to:
// - connect to a firmware server
// - set up ports and terminals,
// - apply levels / thresholds
// - import data segment
// - set up a sequence
// - set measurement mode
// - start measurement
// - find out when measurement is done
// - stop measurement
// - get captured data
// - export captured data to a file
//
// To simplify code the VXI Plug&Play interface is used.
//
// Any error that occurs is logged to stdout or a file.

#include <stdio.h>
#include <stdlib.h>
#include <string.h>

#include "hp81200.h"

#define SYSTEM_NAME1 "DSRA"

#define SETTING_NAME "prog_sample"

static ViSession hInstrument;
static FILE* fp;
```

```
static bool errHandling(ViStatus lStatus, const char *szFctName)
{
    ViChar szErrMsg[hp81200_DEFAULT_BUFFER_SIZE];
    ViInt32 lErrCode;

    if (lStatus != VI_SUCCESS)
    {
        if (lStatus == hp81200_INSTR_ERROR_DETECTED)
        {
            do
            {
                if (hp81200_error_query(hInstrument, &lErrCode, szErrMsg)
                    != VI_SUCCESS)
                {
                    fprintf(fp, "Instrument error: FctName<%s>
                    ErrCode<undetermined> "\
                    "ErrMsg<undetermined>\n", szFctName);
                    break;
                }
            }
            else if (lErrCode != 0)
                fprintf(fp, "Instrument error: FctName<%s> ErrCode<%d>
                ErrMsg<%s>\n",
                szFctName, lErrCode, szErrMsg);
            } while(lErrCode != 0);
        }
        else
        {
            // Not an instrument error

            if (hp81200_error_message(hInstrument, lStatus, szErrMsg)
                != VI_SUCCESS)
                fprintf(fp, "Error: FctName<%s> ErrMsg<undetermined>\n",
                szFctName);
            else
                fprintf(fp, "Error: FctName<%s> ErrMsg<%s>\n", szFctName,
                szErrMsg);
        }
    }
    return (lStatus == VI_SUCCESS);
}
```

```
static bool doIt()
{
    ViChar szParam[hp81200_DEFAULT_BUFFER_SIZE];
    ViChar szAnalyzers[hp81200_DEFAULT_BUFFER_SIZE] = {0};
    ViChar szGenerators[hp81200_DEFAULT_BUFFER_SIZE] = {0};

    ViInt32 lAnalyzerCount = 0;
    ViInt32 lGeneratorCount = 0;
    ViInt32 lAnalyzerPortNumber = 0;
    ViInt32 lGeneratorPortNumber = 0;

    ViStatus lStatus = 0;

    // -----
    // stop system
    // reset system
    // -----

    lStatus = hp81200_systemStop(hInstrument);
    errHandling(lStatus, "hp81200_systemStop");

    lStatus = hp81200_settingNew(hInstrument);
    errHandling(lStatus, "hp81200_settingNew");

    // -----
    // First, we want to generate a list of all analyzers and
    // all generators, so that afterwards we can connect to ports
    // -----

    // Determine number of clock groups
    ViInt32 lClkGeneratorCount;
    lStatus = hp81200_nrOfClockGroups_Q(hInstrument,
    &lClkGeneratorCount);
    errHandling(lStatus, "hp81200_nrOfClockGroups_Q");

    // Loop over all clock groups
    for (ViInt32 c = 1; c <= lClkGeneratorCount; c++)
    {
        ViInt32 lModuleCount;
```

```
// Determine number of modules within this clock group
lStatus = hp81200_nrOfModules_Q(hInstrument, c,
&lModuleCount);
errHandling(lStatus, "hp81200_nrOfModules_Q");

// Loop over all modules
for (ViInt32 m = 1; m <= lModuleCount; m++)
{
    ViInt32 lConnectorCount;
    lStatus = hp81200_nrOfConnectors_Q(hInstrument, c, m,
&lConnectorCount);
    errHandling(lStatus, "hp81200_nrOfConnectors_Q");

    // Loop over all connectors
    for (ViInt32 co = 1; co <= lConnectorCount; co++)
    {
        ViChar szConnectorType[16];
        lStatus = hp81200_typeOfConnector_Q(hInstrument, c, m,
co, szConnectorType);

        errHandling(lStatus, "hp81200_typeOfConnector_Q");

        // Put in analyzer or generator list

        sprintf(szParam, "%02d%02d%03d", c, m, co);
        if (strcmp(szConnectorType, "ANALYZER") == 0)
        {
            // Analyzer
            if (strcmp(szAnalyzers, "") != 0)
                strcat(szAnalyzers, ",");
            strcat(szAnalyzers, szParam);
            lAnalyzerCount ++;
        }
        else
        {
            // Generator
            if (strcmp(szGenerators, "") != 0)
                strcat(szGenerators, ",");
            strcat(szGenerators, szParam);
            lGeneratorCount++;
        }
    }
}
}
```

```
// -----  
// Now connect analyzers and generators to one port each  
// -----  
  
if (lGeneratorCount > 0)  
{  
  
    lStatus = hp81200_portCreation(hInstrument, "DATA",  
    "INPUT_PORT", lGeneratorCount, "input");  
  
    errHandling(lStatus, "hp81200_portCreation");  
    lGeneratorPortNumber = 1;  
    sprintf(szParam, "(%s)", szGenerators);  
    lStatus = hp81200_terminalConnect(hInstrument, "DATA",  
    lGeneratorPortNumber, 1, szParam);  
    errHandling(lStatus, "hp81200_terminalConnect");  
}  
  
if (lAnalyzerCount > 0)  
{  
  
    lStatus = hp81200_portCreation(hInstrument, "DATA",  
    "OUTPUT_PORT", lAnalyzerCount, "output");  
  
    errHandling(lStatus, "hp81200_portCreation");  
    lAnalyzerPortNumber = lGeneratorPortNumber + 1;  
    sprintf(szParam, "(%s)", szAnalyzers);  
  
    lStatus = hp81200_terminalConnect(hInstrument, "DATA",  
    lAnalyzerPortNumber, 1, szParam);  
    errHandling(lStatus, "hp81200_terminalConnect");  
}  
  
// -----  
// Switch on everything, apply levels / thresholds  
// -----  
  
if (lGeneratorPortNumber > 0)  
{  
  
    lStatus = hp81200_portOutputState(hInstrument, "DATA",  
    lGeneratorPortNumber, "ON");  
  
    errHandling(lStatus, "hp81200_portOutputState");  
  
    lStatus = hp81200_portHighLowLevel(hInstrument, "DATA",  
    lGeneratorPortNumber, 2, 0, 0, 50);  
  
    errHandling(lStatus, "hp81200_portHighLowLevel");  
}
```

```
if (lAnalyzerPortNumber > 0)
{
    lStatus = hp81200_portInputState(hInstrument,
    lAnalyzerPortNumber, "ON");
    errHandling(lStatus, "hp81200_portInputState");
    lStatus = hp81200_portInputLevel(hInstrument,
    lAnalyzerPortNumber, 0, 1, 50, 0);
    errHandling(lStatus, "hp81200_portInputLevel");
}

// -----
// Import data (overwrite mode)
// -----
sprintf(szParam, "%s\\samples\\segments\\walk64.txt",
getenv("DVTDSRBASEDIR"));
lStatus = hp81200_segmentLoadFromFile(hInstrument, szParam,
"ON", "");
errHandling(lStatus, "hp81200_segmentLoadFromFile");

// -----
// Set period
// -----
hp81200_systemPeriod(hInstrument, 1E-6);
errHandling(lStatus, "hp81200_systemPeriod");

// -----
// Assign a sequence that uses imported segment
// -----

// Determine number of loop levels available
ViInt32 lLoopLevelCount;
lStatus = hp81200_sequenceAvailableLoopLevel_Q(hInstrument,
&lLoopLevelCount);
errHandling(lStatus, "hp81200_sequenceAvailableLoopLevel_Q");
```

```

// Make infinite loop with trigger using the imported demo
// segment

sprintf(szParam, "(1.0, '', (LOOP%d,1,INF, (BLOCK,0,64",
lLoopLevelCount);
if (lGeneratorPortNumber > 0)
sprintf(szParam, "%s,'walking64',0,0", szParam);

if (lAnalyzerPortNumber > 0)
sprintf(szParam, "%s,'walking64',0,0", szParam);
sprintf(szParam, "%s))", szParam);
lStatus = hp81200_sequence(hInstrument, szParam);
errHandling(lStatus, "hp81200_sequence");

// Generate trigger signal from sequence
lStatus = hp81200_systemTriggerOutSource(hInstrument, 1, "SEQ");
errHandling(lStatus, "hp81200_systemTriggerOutSource");

// -----
// Set measurement mode
// Compare and acquire about error
// -----

if (lAnalyzerPortNumber > 0)
{
    lStatus = hp81200_analyzerErrorCapture(hInstrument, 32768);
    errHandling(lStatus, "hp81200_analyzerErrorCapture");
}

// -----
// Save setting for later use
// -----

lStatus = hp81200_settingSave(hInstrument, SETTING_NAME);
errHandling(lStatus, "hp81200_settingSave");

// -----
// Start measurement
// -----

lStatus = hp81200_systemStart(hInstrument);
errHandling(lStatus, "hp81200_systemStart");

```

```
// -----  
// Poll measurement done  
// THIS ONLY WORKS ONLINE!!!  
// -----  
  
while (true)  
{  
  
    ViChar szExpState[16];  
  
    lStatus = hp81200_systemExpandedState_Q(hInstrument,  
    szExpState);  
  
    errHandling(lStatus, "hp81200_systemExpandedState_Q");  
  
    if (strncmp(szExpState, "FIN", 3) == 0)  
        break;  
  
}  
  
// -----  
// Stop measurement  
// -----  
  
lStatus = hp81200_systemStop(hInstrument);  
errHandling(lStatus, "hp81200_systemStop");  
  
// -----  
// Demonstrate how to deal with captured data  
// Export the captured data and the error memory  
// -----  
  
if (lAnalyzerPortNumber > 0)  
{  
  
    sprintf(szParam, "Analyzer\\Capture.%d",  
    lAnalyzerPortNumber);  
  
    ViInt32 lCaptureInspector;  
  
    lStatus = hp81200_segmentOpen_Q(hInstrument, szParam,  
    &lCaptureInspector);  
  
    errHandling(lStatus, "hp81200_segmentOpen_Q");  
  
    sprintf(szParam, "Analyzer\\ErrMem.%d", lAnalyzerPortNumber);  
  
    ViInt32 lErrMemInspector;  
  
    lStatus = hp81200_segmentOpen_Q(hInstrument, szParam,  
    &lErrMemInspector);  
  
    errHandling(lStatus, "hp81200_segmentOpen_Q");  
  
}
```

```
// Get pattern width (number of traces)
ViInt32 lWidth;

lStatus = hp81200_segmentPatternWidth_Q(hInstrument,
lCaptureInspector,&lWidth);
errHandling(lStatus, "hp81200_PatternWidth_Q");

// Get pattern length (number of vectors)
ViInt32 lLength;

lStatus = hp81200_segmentPatternLength_Q(hInstrument,
lCaptureInspector, &lLength);
errHandling(lStatus, "hp81200_PatternLength_Q");

// Get coding
ViChar szPatternCode[3]; // Possible coding here is only "01"
lStatus = hp81200_segmentPatternCoding_Q(hInstrument,
lCaptureInspector, szPatternCode);
errHandling(lStatus, "hp81200_PatternCoding_Q");

// Write information we got so far:
fprintf(fp, "Analyzer.%d: Coding <%s>, Width %d, Length
%d\n",lAnalyzerPortNumber, szPatternCode, lWidth, lLength);

// Get some data, but assure it does not overflow our small
result-buffer

// To make it human readable, data is returned as a hex
string

if (lLength > 10)
lLength = 10;

if (lLength > 0)
{
// Calculate necessary buffer size
// NOTE: Traces are aligned on byte boundaries
//      Each character (hex digit) uses 4 vectors (with "01"
//      coding)
ViInt32 lHexDigitCount = lLength/4;
if (lLength%4)
// Remaining vectors require another hex digit
lHexDigitCount++;
```

```
// Check if byte-aligned
if (lHexDigitCount%2)
// Byte-align
lHexDigitCount++;
// Count is required for each trace
lHexDigitCount *= lWidth;
ViInt32 lBufferLength = lHexDigitCount+2+1;
ViPChar lpszPattern = (ViPChar)malloc(lBufferLength);
if (lpszPattern == NULL)
{
    fprintf(fp, "Insufficient RAM - run aborted\n" );
    return false;
}
// Take a sample (in hex)
lStatus = hp81200_segmentPatternData_Q(hInstrument,
lCaptureInspector, 0, 0, lWidth-1, lLength-1, lBufferLength,
lpszPattern);
errHandling(lStatus, "hp81200_PatternData_Q");
fprintf(fp, "Analyzer.%d: %s\n", lAnalyzerPortNumber,
lpszPattern);
// Convert data from Hex format to Binary format
// NOTE: Bits within a trace are "from left to right",
//       i.e. first bit is bit 7, then bit 6 and so on
//       for a 1 bit coding
// Display trace-wise
// Divide data into traces
ViInt32 lHexDigitsPerTrace = lHexDigitCount/lWidth;
// Process each trace
for (ViInt32 t = 0; t < lWidth; t++)
{
    fprintf(fp, "Trace %d: ", t);
```

```

// Process each hex digit in trace
for (ViInt32 l = 0; l < lHexDigitsPerTrace; l++)
{
    int nHexDigit;
    ViInt32 lHexDigitIndex = l + (t*lHexDigitsPerTrace);

    if ((*lpszPattern+lHexDigitIndex) >= '0' &&
        (*lpszPattern+lHexDigitIndex) <= '9')
        nHexDigit = *(lpszPattern+lHexDigitIndex) - '0';

    else if ((*lpszPattern+lHexDigitIndex) >= 'A' &&
             (*lpszPattern+lHexDigitIndex) <= 'F')
        nHexDigit = *(lpszPattern+lHexDigitIndex) - 'A' +
            10;

    else
        // Illegal digit - ignore
        nHexDigit = 0;

    // Process each bit (vector) in hex digit
    for (int v = 3; v >= 0; v--)
    {
        if ((l*4) + (4-v) > lLength)
            // Ignore padding required for byte-alignment
            // break;

        if (nHexDigit / (1 << v))
        {
            // Bit is set
            fprintf(fp, "1");

            // Set bit has been treated => remove it
            nHexDigit -= (1 << v);
        }
        else
            // Bit is not set
            fprintf(fp, "0");
    }
    fprintf(fp, "\n");
}

// Pattern buffer can now be discarded
free(lpszPattern);
}

```

```
// Save segments under a different name to the local setting
lStatus = hp81200_segmentSave(hInstrument, lCaptureInspector,
"LocalSegments\\prog_sample_capture");

errHandling(lStatus, "hp81200_segmentSave");

lStatus = hp81200_segmentSave(hInstrument, lErrMemInspector,
"LocalSegments\\prog_sample_errmem");

errHandling(lStatus, "hp81200_segmentSave");

// Export segments
// This is done now before the segments are closed, because
// they are now still in memory

lStatus = hp81200_segmentSaveToFile(hInstrument,
"c:\\temp\\prog_sample_capture.txt", SETTING_NAME,
"prog_sample_capture");

errHandling(lStatus, "hp81200_segmentSaveToFile");

lStatus = hp81200_segmentSaveToFile(hInstrument,
"c:\\temp\\prog_sample_errmem.txt", SETTING_NAME,
"prog_sample_errmem");

errHandling(lStatus, "hp81200_segmentSaveToFile");

// Close the segments!

lStatus = hp81200_segmentClose(hInstrument, lCaptureInspector);
errHandling(lStatus, "hp81200_segmentClose");

lStatus = hp81200_segmentClose(hInstrument, lErrMemInspector);
errHandling(lStatus, "hp81200_segmentClose");

}

return true;
}

int main()
{
    ViStatus lStatus = 0;

    ViBoolean bIDQuery = VI_FALSE;
    ViBoolean bResetDevice = VI_FALSE;

    ViString szSystemNameHp81200 = SYSTEM_NAME1;
    ViString szApplicationName = "DSR";
```

```
// Errors are logged to a file (which may be stdout).
//fp = fopen("c:\\temp\\sample_4.txt", "w");
fp = stdout;

// Initialize the software connection to the 81200 system
lStatus = hp81200_init("VXI0::0::INSTR", bIDQuery, bResetDevice,
&hInstrument );
errHandling(lStatus, "hp81200_init");

// For remote access
lStatus = hp81200_connect(hInstrument, "fox00099", "2203");
errHandling(lStatus, "hp81200_connect");
lStatus = hp81200_systemSelect(hInstrument, szSystemNameHp81200,
szApplicationName);
errHandling(lStatus, "hp81200_systemSelect");
fprintf(fp, "System %s:\n", szSystemNameHp81200);
doIt();

hp81200_close(hInstrument);

// Wait so that user can see the results
if ((fp == stdout) || (fp == stderr))
{
    printf("Press any key to continue\n");
    (void)getchar();
}
else
fclose(fp);

return (lStatus != VI_SUCCESS);
// (TRUE) 1 => failure, (FALSE) 0 => success
}
```

Lib.cpp Interface Class Library Code

The following code provides the library functions for initializing the system, dealing with handles, executing the SCPI commands, and logging errors.

```
//
// small interface class to the 81200A
//
// provides error logging, handle-handling
//
// This example is limited in functionality, because there
// are fixed command and response buffers.
//

#include <ctype.h>
#include <string.h>
#include <hp81200.h>

#include "lib.h"

// init
HP81200::HP81200()
: itsErrorFile(0), itsConnected(false)
{
    strcpy(itsHandle, "");
    strcpy(itsResultBuffer, "");
}

// make sure we released handle and disconnected from the system
HP81200::~HP81200()
{
    // assure that handle is destroyed...
    if (strcmp(itsHandle, "") != 0)
        (void)Exit();
}

// Connect to 81200 server on local machine or "theServerName".
// Creates a handle for the system "theSystemName".
// This handle is internally handled, so that we do not need
// to specify it with each command.
bool HP81200::Init( const char* theServerName,
                   const char* theHandleSuggestion,
                   const char* theSystemName,
                   FILE* theErrorFile)
```

```

{
    bool b;
    char aCmd[128];
    int ret;

    // remember error log file
    itsErrorFile = theErrorFile;

    // connect to firmware server
    // if already connected do nothing
    ret = Connect_HP81200(theServerName);
    itsConnected = (ret == 0);
    if (!itsConnected && (ret != -4))
    {
        WriteErrorLog(ret);
        return false;
    }

    // create a handle
    sprintf(aCmd, ":dvt:inst:hand:cre? %s,'DSR','%s'",
        theHandleSuggestion, theSystemName);
    b = Call(aCmd);

    strcpy(itsHandle, itsResultBuffer);

    return b;
}

// Release the handle, disconnect from the system
bool HP81200::Exit()
{
    if (strcmp(itsHandle, "") != 0)
    {
        bool b;
        char aCmd[128];

        // destroy handle
        sprintf(aCmd, ":dvt:inst:hand:dest %s", itsHandle);
        b = Call(aCmd);
        if (!b) return b;

        // clear remembered handle
        strcpy(itsHandle, "");
    }

    if (itsConnected)
    {
        int ret;

        ret = Disconnect_HP81200();
        if (ret != 0)
        {

```

```

        WriteErrorLog(ret);
        return false;
    }
}

return true;
}

// Call 81200, handle is automatically supplied by the class.
// Errors are logged to the logfile.
// In case of an error, false is returned.
// Results from the call are ignored.
bool HP81200::Call(const char* theCmd)
{
    int ret;
    char aCmd[1024];
    int aResultLen;

    if (strcmp(GetHandle(theCmd), "dvt") == 0)
        // already valid command with handle dvt, just use it...
        sprintf(aCmd, "%s", theCmd);
    else if (theCmd[0] == ':')
        // command for local handle
        sprintf(aCmd, ":%s%s", itsHandle, theCmd);
    else
        // command for local handle
        sprintf(aCmd, ":%s:%s", itsHandle, theCmd);

    aResultLen = sizeof(itsResultBuffer);
    ret = Call_HP81200(aCmd, itsResultBuffer, &aResultLen);
    if (ret != 0)
    {
        WriteErrorLog(ret, theCmd);
        return false;
    }

    return true;
}

// Call 81200, handle is automatically supplied by the class.
// Errors are logged to the logfile.
// In case of an error, false is returned.
// Results are returned as a pointer to an internal buffer,
// so before calling Call again, the results must be otherwise
// saved.
bool HP81200::Call(const char* theCmd, const char*& theResult)
{
    theResult = itsResultBuffer;

    return Call(theCmd);
}

```

```

// extract handle part of a command string (private method)
const char* HP81200::GetHandle(const char* theCmd)
{
    if (theCmd == 0)
        return itsHandle;
    else if ((theCmd[0] == ':' ) &&
        (tolower(theCmd[1]) == 'd') &&
        (tolower(theCmd[2]) == 'v') &&
        (tolower(theCmd[3]) == 't'))
        // already valid command vor dvt-handle
        return "dvt";
    else if ((tolower(theCmd[0]) == 'd') &&
        (tolower(theCmd[1]) == 'v') &&
        (tolower(theCmd[2]) == 't'))
        // already valid command vor dvt-handle
        return "dvt";
    else if (theCmd[0] == ':')
        return itsHandle;
    else
        return itsHandle;
}

// write to error log file (private method)
void HP81200::WriteErrorLog(int theRet, const char* theCmd)
{
    if (itsErrorFile != 0)
    {
        char aErrorStr[1024];
        int aErrorLen = sizeof(aErrorStr);

        // write header for the error
        if (theCmd != 0)
            fprintf(itsErrorFile, "Error for cmd <%s>\n", theCmd);

        if (theRet < 0)
        {
            // get and print error message corresponding
            // to the return value
            GetErrStr_HP81200(theRet, aErrorStr, &aErrorLen);
            fprintf(itsErrorFile, "\t%s\n", aErrorStr);
        }
        else
        {
            // get and print error message from the error queue
            char aResultBuffer[1024];
            int aResultLen;
            char aCmd[128];

            sprintf(aCmd, ":%s:syst:err?", GetHandle(theCmd));
            for (;;)
            {

```

```
        aResultLen = sizeof(aResultBuffer);
        int ret = Call_HP81200(aCmd, aResultBuffer,
                               &aResultLen);

        // break out of loop if error queue empty
        if ((ret != 0) || (aResultBuffer[0] == '0'))
            break;

        fprintf(itsErrorFile, "\t%s\n", aResultBuffer);
    }
}
}
```

Main.cpp Application Code

The following code is a typical example program for accessing the user software functionality.

```
// main.cpp
// This is a small demo program showing how to use
// the remote interface of the 81200A
// user software
//
// It demonstrates how to:
// - connect to a firmware server
// - set up ports and terminals,
// - apply levels / thresholds
// - import data segment
// - set up a sequence
// - set measurement mode
// - start measurement
// - find out when measurement is done
// - stop measurement
// - get captured data
// - export captured data to a file
//
// to make this code easier to read,
// it is based on a small class HP81200
// which is provided in lib.c / lib.h
// Here the error handling and the "handle" is hidden.
// Any error that occurs is logged to stdout or file.
//

#include <stdio.h>
#include <stdlib.h>
#include <string.h>

#include "lib.h"

#define SYSTEM_NAME1 "DSRA"

#define SETTING_NAME "prog_sample"

static bool doIt(HP81200& h, FILE* fp)
{
    const char* aResult;
    char aCmd[4096];
    char aBuf[1024];
    char aAnalyzers[1024];
```

```

char aGenerators[1024];
int aAnaCnt;
int aGenCnt;
int aAnaPort;
int aGenPort;

// -----
// stop system
// reset system
// -----
h.Call("sgen:glob:init:cont off");
h.Call("mmem:sett:new");

// -----
// first, we want to generate a list of all analyzers and
// all generators, so that we can afterwards connect to ports
// -----
strcpy(aAnalyzers, "");
strcpy(aGenerators, "");
aAnaCnt = 0;
aGenCnt = 0;
aAnaPort = 0;
aGenPort = 0;

// find out how many clock groups we have
h.Call("conf:cgr?", aResult);
int aCgr;
sscanf(aResult, "%d", &aCgr);

// loop over all clock groups
for (int c = 1; c <= aCgr; c++)
{
    // find out how many modules within this clock group
    sprintf(aCmd, "conf:cgr%d:mod?", c);
    h.Call(aCmd, aResult);
    int aMod;
    sscanf(aResult, "%d", &aMod);

    // loop over all modules
    for (int m = 1; m <= aMod; m++)
    {
        // find out how many connectors we have...
        sprintf(aCmd, "conf:cgr%d:mod%d:conn?", c, m);
        h.Call(aCmd, aResult);
        int aConn;
        sscanf(aResult, "%d", &aConn);

        // loop over connectors
        for (int co = 1; co <= aConn; co++)

```

```

    {
        // query for type
        sprintf(aCmd, "conf:cgr%d:mod%d:conn%d:type?", c, m,
            co);
        h.Call(aCmd, aResult);

        // put to analyzer or generator list
        sprintf(aBuf, "%02d%02d%03d", c, m, co);
        if (strcmp(aResult, "ANALYZER") == 0)
        {
            if (strcmp(aAnalyzers, "") != 0)
                strcat(aAnalyzers, ",");
            strcat(aAnalyzers, aBuf);
            aAnaCnt += 1;
        }
        else
        {
            if (strcmp(aGenerators, "") != 0)
                strcat(aGenerators, ",");
            strcat(aGenerators, aBuf);
            aGenCnt += 1;
        }
    }
}

// -----
// now connect analyzers and generators to one port each
// -----
if (aGenCnt > 0)
{
    sprintf(aCmd, "sgen:pdat:app 'INPUT_PORT',%d,'input'",
        aGenCnt);
    h.Call(aCmd);

    aGenPort = 1;
    sprintf(aCmd, "sgen:conn:pdat%d:term1 (@%s)", aGenPort,
        aGenerators);
    h.Call(aCmd);
}

if (aAnaCnt > 0)
{
    sprintf(aCmd, "sgen:pdat:app 'OUTPUT_PORT',%d,'output'",
        aAnaCnt);
    h.Call(aCmd);

    aAnaPort = aGenPort + 1;
    sprintf(aCmd, "sgen:conn:pdat%d:term1 (@%s)", aAnaPort,
        aAnalyzers);
    h.Call(aCmd);
}

```

```

// -----
// switch on everything, apply levels / thresholds
// -----
if (aGenPort > 0)
{
    sprintf(aCmd, "sgen:pdat%d:outp on", aGenPort);
    h.Call(aCmd);

    sprintf(aCmd, "sgen:pdat%d:volt:high 2", aGenPort);
    h.Call(aCmd);
}

if (aAnaPort > 0)
{
    sprintf(aCmd, "sgen:pdat%d:inp on", aAnaPort);
    h.Call(aCmd);

    sprintf(aCmd, "sgen:pdat%d:inp:thr 1", aAnaPort);
    h.Call(aCmd);
}

// -----
// import data (overwrite mode)
// -----
sprintf(aCmd,
        "mmem:segm:load '%s\\samples\\segments\\walk64.txt'",
        getenv("DVTDSRBASEDIR"));
h.Call(aCmd);

// -----
// set period
// -----
h.Call("sgen:glob:per 1e-6");

// -----
// assign a sequence that uses imported segment
// -----

// how many loop levels are available?
h.Call("sgen:glob:seq:llev?", aResult);
int aLoopLevels = 0;
sscanf(aResult, "%d", &aLoopLevels);

// make infinite loop with trigger using the imported
// demo segment
sprintf(aCmd,
        "sgen:glob:seq (1.0,'',(LOOP%d,1,INF,(BLOCK,0,64",

```

```

        aLoopLevels);
if (aGenPort > 0)
    sprintf(aCmd, "%s,'walking64',0,0", aCmd);
if (aAnaPort > 0)
    sprintf(aCmd, "%s,'walking64',0,0", aCmd);
sprintf(aCmd, "%s)))", aCmd);
h.Call(aCmd);

// generate trigger signal from sequence
h.Call("cgr:trig:mode seq");

// -----
// set measurement mode
// compare and acquire around error
// -----
if (aAnaPort > 0)
    h.Call("sgen:glob:conf:ecap");

// -----
// save setting for later use
// -----
sprintf(aCmd, "mmem:sett:save '%s'", SETTING_NAME);
h.Call(aCmd);

// -----
// start measurement
// -----
h.Call("sgen:glob:init:cont on");

// -----
// poll measurement done
// THIS ONLY WORKS ONLINE!!!
// -----
for (;;)
{
    h.Call("sgen:glob:syst:stat?", aResult);
    if (strncmp(aResult, "FIN", 3) == 0)
        break;
}

// -----
// stop measurement
// -----
h.Call("sgen:glob:init:cont off");

// -----
// - demonstrate the edit subsystem how to deal with
//   captured data
// - export the captured data and the error memory

```

```

// -----
if (aAnaPort > 0)
{
    sprintf(aCmd, "edit:segm:open? `Analyzer\\Capture.%d'",
            aAnaPort);
    h.Call(aCmd, aResult);
    int aCapture;
    sscanf(aResult, "%d", &aCapture);

    sprintf(aCmd, "edit:segm:open? `Analyzer\\ErrMem.%d'",
            aAnaPort);
    h.Call(aCmd, aResult);
    int aErrMem;
    sscanf(aResult, "%d", &aErrMem);

    // get pattern width
    sprintf(aCmd, "edit:segm%d:patt:widt?", aCapture);
    h.Call(aCmd, aResult);
    int aWidth;
    sscanf(aResult, "%d", &aWidth);

    // get pattern length
    sprintf(aCmd, "edit:segm%d:patt:leng?", aCapture);
    h.Call(aCmd, aResult);
    int aLength;
    sscanf(aResult, "%d", &aLength);

    // get Coding
    sprintf(aCmd, "edit:segm%d:patt:cod?", aCapture);
    h.Call(aCmd, aResult);

    // write information we got so far:
    fprintf(fp, "Analyzer.%d: Coding <%=s>,
            Width %d, Length %d\n",
            aAnaPort, aResult, aWidth, aLength);

    // get some data, but assure that we will not overflow our
    // small result-buffer
    // to make it human readable, we get the data as a hex-string
    if (aLength > 10) aLength = 10;
    if (aLength > 0)
    {
        sprintf(aCmd, "edit:segm%d:patt:data? 0,0,%d,%d,HEX",
                aCapture, aWidth-1, aLength-1);
        h.Call(aCmd, aResult);
        fprintf(fp, "Analyzer.%d: %s\n", aAnaPort, aResult);
    }

    //
    // extract the vectors and print as '0' and '1' to fp

```

```

//

// get vector data as definite length block
sprintf(aCmd, "edit:segm%d:patt:data? 0,0,%d,%d,BIN",
        aCapture, aWidth-1, aLength-1);
h.Call(aCmd, aResult);

// extract raw data from definite length block
// a definite length block looks like
// #d11111bbbbbbbb
// where d is the number of length digits 1
// then length binary bytes b are following
// Example: #90000000012xxxxxxxxxxxx
// where x stands for any value between 0 and 255,
// it may not be a readable character!
memcpy(aBuf, &aResult[2], (size_t)(aResult[1] - '0'));
aBuf[aResult[1]] = '\0';
int aBytes = 0;
sscanf(aBuf, "%d", &aBytes);
memcpy(aBuf, &aResult[2+aResult[1]-'0'], (size_t)aBytes);

// print out the data trace-wise
// - each trace begins on a byte boundary
// - bits within a trace are "from left to right",
//   meaning that first bit is bit 7, than bit 6
//   and so on for a 1 bit coding.
for (int t = 0; t < aWidth; t++)
{
    fprintf(fp, "Trace %d: ", t);
    for (int l = 0; l < aLength; l++)
    {
        fprintf(fp, "%c", '0' +
                ((aBuf[t * ((aLength+7)/8) + l/8] >> (7 - l%8)) & 1)
                );
    }
    fprintf(fp, "\n");
}

// save segments under a different name to the local setting
sprintf(aCmd,
        "edit:segm%d:save 'LocalSegments\\prog_sample_capture'",
        aCapture);
h.Call(aCmd);
sprintf(aCmd,
        "edit:segm%d:save 'LocalSegments\\prog_sample_errmem'",
        aErrMem);
h.Call(aCmd);

```

```

        // export segments
        // we do this now before the segments are closed, because
        // they are now still in memory
        sprintf(aCmd,
            "mmem:segm:save 'c:\\temp\\prog_sample_capture.txt', '%s',
            'prog_sample_capture'", SETTING_NAME);
        h.Call(aCmd);

        sprintf(aCmd,
            "mmem:segm:save 'c:\\temp\\prog_sample_errmem.txt', '%s',
            'prog_sample_errmem'", SETTING_NAME);
        h.Call(aCmd);

        // don't forget to close the segments again!
        sprintf(aCmd, "edit:segm%d:clos", aCapture);
        h.Call(aCmd);

        sprintf(aCmd, "edit:segm%d:clos", aErrMem);
        h.Call(aCmd);
    }

    return true;
}

int main()
{
    bool b;
    HP81200 a;
    FILE* fp;

    //fp = fopen("c:\\temp\\sample_4.txt", "w");
    fp = stdout;

    // init access to local 81200 firmware server, system "DSRA"
    // Errors are logged to a file (which may be stdout).
    b = a.Init("", "a", SYSTEM_NAME1, fp);
    if (b) {
        fprintf(fp, "System %s:\n", SYSTEM_NAME1);
        b = doIt(a, fp);
    }

    // release handle, disconnect from server
    (void)a.Exit();

    // wait, so that user could see the results
    if ((fp == stdout) || (fp == stderr))
    {

```

```

        printf("press any key to continue\n");
        (void)getchar();
    }
    else
        fclose(fp);

    return 0;
}

// Connect to 81200 server on local machine or "theServerName".
// Creates a handle for the system "theSystemName".
// This handle is internally handled, so that we do not need
// to specify it with each command.
bool HP81200::Init( const char* theServerName,
                  const char* theHandleSuggestion,
                  const char* theSystemName,
                  FILE* theErrorFile)
{
    bool b;
    char aCmd[128];
    int ret;

    // remember error log file
    itsErrorFile = theErrorFile;

    // connect to firmware server
    // if already connected do nothing
    ret = Connect_HP81200(theServerName);
    itsConnected = (ret == 0);
    if (!itsConnected && (ret != -4))
    {
        WriteErrorLog(ret);
        return false;
    }

    // create a handle
    sprintf(aCmd, ":dvt:inst:hand:cre? %s,'DSR','%s'",
          theHandleSuggestion, theSystemName);
    b = Call(aCmd);

    strcpy(itsHandle, itsResultBuffer);

    return b;
}

// Release the handle, disconnect from the system
bool HP81200::Exit()
{
    if (strcmp(itsHandle, "") != 0)
    {
        bool b;
        char aCmd[128];
    }
}

```

```

        // destroy handle
        sprintf(aCmd, ":dvt:inst:hand:dest %s", itsHandle);
        b = Call(aCmd);
        if (!b) return b;

        // clear remembered handle
        strcpy(itsHandle, "");
    }

    if (itsConnected)
    {
        int ret;

        ret = Disconnect_HP81200();
        if (ret != 0)
        {
            WriteErrorLog(ret);
            return false;
        }
    }

    return true;
}

// Call 81200, handle is automatically supplied by the class.
// Errors are logged to the logfile.
// In case of an error, false is returned.
// Results from the call are ignored.
bool HP81200::Call(const char* theCmd)
{
    int ret;
    char aCmd[1024];
    int aResultLen;

    if (strcmp(GetHandle(theCmd), "dvt") == 0)
        // already valid command with handle dvt, just use it...
        sprintf(aCmd, "%s", theCmd);
    else if (theCmd[0] == ':')
        // command for local handle
        sprintf(aCmd, ":%s%s", itsHandle, theCmd);
    else
        // command for local handle
        sprintf(aCmd, ":%s:%s", itsHandle, theCmd);

    aResultLen = sizeof(itsResultBuffer);
    ret = Call_HP81200(aCmd, itsResultBuffer, &aResultLen);
    if (ret != 0)
    {
        WriteErrorLog(ret, theCmd);
        return false;
    }
}

```

```

        return true;
    }

    // Call 81200, handle is automatically supplied by the class.
    // Errors are logged to the logfile.
    // In case of an error, false is returned.
    // Results are returned as a pointer to an internal buffer,
    // so before calling Call again, the results must be otherwise
    // saved.
bool HP81200::Call(const char* theCmd, const char*& theResult)
{
    theResult = itsResultBuffer;

    return Call(theCmd);
}

int main()
{
    bool b;
    HP81200 a;
    FILE* fp;

    //fp = fopen("c:\\temp\\sample_4.txt", "w");
    fp = stdout;

    // init access to local 81200 firmware server, system "DSRA"
    // Errors are logged to a file (which may be stdout).
    b = a.Init("", "a", SYSTEM_NAME1, fp);
    if (b) {
        fprintf(fp, "System %s:\n", SYSTEM_NAME1);
        b = doIt(a, fp);
    }

    // release handle, disconnect from server
    (void)a.Exit();

    // wait, so that user could see the results
    if ((fp == stdout) || (fp == stderr))
    {
        printf("press any key to continue\n");
        (void)getchar();
    }
    else
        fclose(fp);

    return 0;
}

```

```

// -----
// stop system
// reset system
// -----
h.Call("sgen:glob:init:cont off");
h.Call("mmem:sett:new");

// -----
// first, we want to generate a list of all analyzers and
// all generators, so that we can afterwards connect to ports
// -----
strcpy(aAnalyzers, "");
strcpy(aGenerators, "");
aAnaCnt = 0;
aGenCnt = 0;
aAnaPort = 0;
aGenPort = 0;

// find out how many clock groups we have
h.Call("conf:cgr?", aResult);
int aCgr;
sscanf(aResult, "%d", &aCgr);

// loop over all clock groups
for (int c = 1; c <= aCgr; c++)
{
    // find out how many modules within this clock group
    sprintf(aCmd, "conf:cgr%d:mod?", c);
    h.Call(aCmd, aResult);
    int aMod;
    sscanf(aResult, "%d", &aMod);

    // loop over all modules
    for (int m = 1; m <= aMod; m++)
    {
        // find out how many connectors we have...
        sprintf(aCmd, "conf:cgr%d:mod%d:conn?", c, m);
        h.Call(aCmd, aResult);
        int aConn;
        sscanf(aResult, "%d", &aConn);

        // loop over connectors
        for (int co = 1; co <= aConn; co++)
        {
            // query for type
            sprintf(aCmd, "conf:cgr%d:mod%d:conn%d:type?", c, m,
                co);
            h.Call(aCmd, aResult);

            // put to analyzer or generator list
            sprintf(aBuf, "%02d%02d%03d", c, m, co);

```

```

        if (strcmp(aResult, "ANALYZER") == 0)
        {
            if (strcmp(aAnalyzers, "") != 0)
                strcat(aAnalyzers, ",");
            strcat(aAnalyzers, aBuf);
            aAnaCnt += 1;
        }
        else
        {
            if (strcmp(aGenerators, "") != 0)
                strcat(aGenerators, ",");
            strcat(aGenerators, aBuf);
            aGenCnt += 1;
        }
    }
}

// -----
// now connect analyzers and generators to one port each
// -----
if (aGenCnt > 0)
{
    sprintf(aCmd, "sgen:pdat:app 'INPUT_PORT',%d,'input'",
            aGenCnt);
    h.Call(aCmd);

    aGenPort = 1;
    sprintf(aCmd, "sgen:conn:pdat%d:term1 (@%s)", aGenPort,
            aGenerators);
    h.Call(aCmd);
}

if (aAnaCnt > 0)
{
    sprintf(aCmd, "sgen:pdat:app 'OUTPUT_PORT',%d,'output'",
            aAnaCnt);
    h.Call(aCmd);

    aAnaPort = aGenPort + 1;
    sprintf(aCmd, "sgen:conn:pdat%d:term1 (@%s)", aAnaPort,
            aAnalyzers);
    h.Call(aCmd);
}

// -----
// switch on everything, apply levels / thresholds
// -----
if (aGenPort > 0)
{
    sprintf(aCmd, "sgen:pdat%d:outp on", aGenPort);
    h.Call(aCmd);
}

```

```

        sprintf(aCmd, "sgen:pdat%d:volt:high 2", aGenPort);
        h.Call(aCmd);
    }

    if (aAnaPort > 0)
    {
        sprintf(aCmd, "sgen:pdat%d:inp on", aAnaPort);
        h.Call(aCmd);

        sprintf(aCmd, "sgen:pdat%d:inp:thr 1", aAnaPort);
        h.Call(aCmd);
    }

    // -----
    // import data (overwrite mode)
    // -----
    sprintf(aCmd,
        "mmem:segm:load '%s\\samples\\segments\\walk64.txt'",
        getenv("DVTDSRBASEDIR"));
    h.Call(aCmd);

    // -----
    // set period
    // -----
    h.Call("sgen:glob:per 1e-6");

    // -----
    // assign a sequence that uses imported segment
    // -----

    // how many loop levels are available?
    h.Call("sgen:glob:seq:llev?", aResult);
    int aLoopLevels = 0;
    sscanf(aResult, "%d", &aLoopLevels);

    // make infinite loop with trigger using the imported
    // demo segment
    sprintf(aCmd,
        "sgen:glob:seq (1.0,'',(LOOP%d,1,INF,(BLOCK,0,64",
        aLoopLevels);
    if (aGenPort > 0)
        sprintf(aCmd, "%s,'walking64',0,0", aCmd);
    if (aAnaPort > 0)
        sprintf(aCmd, "%s,'walking64',0,0", aCmd);
    sprintf(aCmd, "%s)))", aCmd);
    h.Call(aCmd);

    // generate trigger signal from sequence
    h.Call("cgr:trig:mode seq");

```

```

// -----
// set measurement mode
// compare and acquire around error
// -----
if (aAnaPort > 0)
    h.Call("sgen:glob:conf:ecap");

// -----
// save setting for later use
// -----
sprintf(aCmd, "mmem:sett:save '%s'", SETTING_NAME);
h.Call(aCmd);

// -----
// start measurement
// -----
h.Call("sgen:glob:init:cont on");

// -----
// poll measurement done
// THIS ONLY WORKS ONLINE!!!
// -----
for (;;)
{
    h.Call("sgen:glob:syst:stat?", aResult);
    if (strncmp(aResult, "FIN", 3) == 0)
        break;
}

// -----
// stop measurement
// -----
h.Call("sgen:glob:init:cont off");

// -----
// - demonstrate the edit subsystem how to deal with
//   captured data
// - export the captured data and the error memory
// -----
if (aAnaPort > 0)
{
    sprintf(aCmd, "edit:segm:open? 'Analyzer\\Capture.%d'",
            aAnaPort);
    h.Call(aCmd, aResult);
    int aCapture;
    sscanf(aResult, "%d", &aCapture);

    sprintf(aCmd, "edit:segm:open? 'Analyzer\\ErrMem.%d'",
            aAnaPort);
    h.Call(aCmd, aResult);
}

```

```

int aErrMem;
sscanf(aResult, "%d", &aErrMem);

// get pattern width
sprintf(aCmd, "edit:segm%d:patt:widt?", aCapture);
h.Call(aCmd, aResult);
int aWidth;
sscanf(aResult, "%d", &aWidth);

// get pattern length
sprintf(aCmd, "edit:segm%d:patt:leng?", aCapture);
h.Call(aCmd, aResult);
int aLength;
sscanf(aResult, "%d", &aLength);

// get Coding
sprintf(aCmd, "edit:segm%d:patt:cod?", aCapture);
h.Call(aCmd, aResult);

// write information we got so far:
fprintf(fp, "Analyzer.%d: Coding <%s>,
          Width %d, Length %d\n",
          aAnaPort, aResult, aWidth, aLength);

// get some data, but assure that we will not overflow our
// small result-buffer
// to make it human readable, we get the data as a hex-string
if (aLength > 10) aLength = 10;
if (aLength > 0)
{
    sprintf(aCmd, "edit:segm%d:patt:data? 0,0,%d,%d,HEX",
            aCapture, aWidth-1, aLength-1);
    h.Call(aCmd, aResult);
    fprintf(fp, "Analyzer.%d: %s\n", aAnaPort, aResult);

    //
    // extract the vectors and print as '0' and '1' to fp
    //

    // get vector data as definite length block
    sprintf(aCmd, "edit:segm%d:patt:data? 0,0,%d,%d,BIN",
            aCapture, aWidth-1, aLength-1);
    h.Call(aCmd, aResult);

    // extract raw data from definite length block
    // a definite length block looks like
    // #d11111bbbbbbbbb
    // where d is the number of length digits 1
    // then length binary bytes b are following

```

```

// Example: #90000000012xxxxxxxxxxxxx
// where x stands for any value between 0 and 255,
// it may not be a readable character!
memcpy(aBuf, &aResult[2], (size_t)(aResult[1] - '0'));
aBuf[aResult[1]] = '\0';
int aBytes = 0;
sscanf(aBuf, "%d", &aBytes);
memcpy(aBuf, &aResult[2+aResult[1]-'0'], (size_t)aBytes);

// print out the data trace-wise
// - each trace begins on a byte boundary
// - bits within a trace are "from left to right",
// meaning that first bit is bit 7, than bit 6
// and so on for a 1 bit coding.
for (int t = 0; t < aWidth; t++)
{
    fprintf(fp, "Trace %d: ", t);
    for (int l = 0; l < aLength; l++)
    {
        fprintf(fp, "%c", '0' +
            ((aBuf[t * ((aLength+7)/8) + l/8] >> (7 - l%8)) & 1)
        );
    }
    fprintf(fp, "\n");
}
}

// save segments under a different name to the local setting
sprintf(aCmd,
    "edit:segm%d:save 'LocalSegments\\prog_sample_capture'",
    aCapture);
h.Call(aCmd);
sprintf(aCmd,
    "edit:segm%d:save 'LocalSegments\\prog_sample_errmem'",
    aErrMem);
h.Call(aCmd);

// export segments
// we do this now before the segments are closed, because
// they are now still in memory
sprintf(aCmd,
    "mmem:segm:save 'c:\\temp\\prog_sample_capture.txt', '%s',
    'prog_sample_capture'", SETTING_NAME);
h.Call(aCmd);

sprintf(aCmd,
    "mmem:segm:save 'c:\\temp\\prog_sample_errmem.txt', '%s',
    'prog_sample_errmem'", SETTING_NAME);
h.Call(aCmd);

```

```
        // don't forget to close the segments again!  
        sprintf(aCmd, "edit:segm%d:clos", aCapture);  
        h.Call(aCmd);  
  
        sprintf(aCmd, "edit:segm%d:clos", aErrMem);  
        h.Call(aCmd);  
    }  
}
```


Copyright Agilent Technologies 2006
Printed in Germany March 2006



5988-4886EN



Agilent Technologies