

Agilent OmniBER OTN Family

OmniBER OTN
communications
performance analyzer

Quick Reference Guide



Agilent Technologies



**Agilent
OmniBER OTN
Family**

**Quick Reference
Guide**



Notices

© 2003 Agilent Technologies UK Limited

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Agilent Technologies UK Limited as governed by international copyright laws.

Manual Part Number

J7230-90053

Edition

First edition, August 2003

Printed in UK

Agilent Technologies UK Limited

Data Networks Division

South Queensferry, West Lothian, Scotland
EH30 9TG

Sales and Service Offices

An up-to-date list of Agilent Offices is available through the Agilent Website at URL: <http://www.agilent.com>

Warranty

The material contained in this document is provided "as is," and is subject to being changed without notice in future editions. Further, to the maximum extent permitted by applicable law, Agilent Technologies disclaims all warranties of merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any of the products to which it pertains. Should Agilent Technologies have a written contract with the user and should any of the contract terms conflict with these terms the contract terms shall control.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or sub-contract, Software is delivered and licensed as "Commercial computer software" as defined in DFAR 252.227-7014 (June 1995), or as a "commercial item" as defined in FAR 2.101(a) or as "Restricted computer software" as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies' standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

In This Quick Reference Guide...

This guide contains:

- The conventions used within this guide.
- A guide to the instrument's front panel and the Graphical User Interface (GUI).
- Information on how to get help, including an introduction to the Online Help, what is in it and how to use it.
- Quick reference tables to help you quickly select the major instrument functions.

Conventions Used in This Guide...

- Front panel buttons appear in bold within angled brackets. For example, press **<Menu>**.
- When buttons are connected by a plus (+) sign, for example, **<2> + <4>**, press the listed buttons in sequence.
- Menu items appear in bold. The greater than (>) symbol separates each menu level. For example, **'Test Functions > Errors and Alarms'** indicates that you should choose 'Errors and Alarms' from the 'Test Functions' main menu.
- This Guide applies to SONET, SDH, OTN, PDH and DS_n network standards.

Contents

1 Product Introduction

- Introduction 8
- New Features 8

2 Getting Help

- Accessing the Online Help 10
 - What is in the Online Help? 10
- Which Keys Do I Press? 11
- Accessing the Index 11
- Creating/Accessing Your Own Help Files 12
- Installation Manual 13
- User Resources on the CD-ROM 13

3 Quick Reference Tables

- Smart Test 16
- Transmitter Functions 17
- Receiver Functions 19
- Results 20
- Test Functions 22
- Overhead Monitor 23
- Overhead Setup 24
- System Functions 25
- System Functions – File Manager 26
- Print Control 27



1 Product Introduction

Introduction 8

New Features 8

For a full list of specifications, see the technical specifications document, available on the instrument webpage, URL:

http://www.agilent.com/comms/otn_jitter

or

http://www.agilent.com/comms/otn_2-5g



Introduction

The OmniBER OTN family provides a rich feature-set for the development and testing of equipment designed for the Optical Transport Network (OTN G.709), plus the capability for jitter and wander testing, SONET/SDH testing, PDH/DSn testing and next generation SONET/SDH (GFP/LAPS) payload testing.

For more detailed product information, see the OmniBER OTN Family brochure, available on the product website:
<http://www.agilent.com/comms/otn>



New Features

In addition to the standard OmniBER OTN features, these instruments offer the following new features:

J7232A (2.5 Gb/s)

- GFP/LAPS Ethernet MAC payload testing
- PDH/DSn testing at all rates from 1.5 Mb/s to 2.5 Gb/s

J7231B (10 Gb/s)

- Jitter/wander testing at all optical rates
- Jitter/wander tolerance testing
- Jitter transfer testing
- PDH/DSn tributary testing



2 Getting Help

Accessing the Online Help	10
What is in the Online Help?	10
Which Keys Do I Press?	11
Accessing the Index	11
Creating/Accessing Your Own Help Files	12
Installation Manual	13
User Resources on the CD-ROM	13

You can get help from the Online Help on the instrument, the CD-ROM or the Installation manual.

The Online Help explains how to set up and use the instrument. It also contains a Getting Started section for new users, which includes measurement tutorials to help you learn how to use the instrument.

Also, you will find a comprehensive index and glossary, plus a Telecoms Concepts section with telecoms reference information. You can add your own help files (in HTML format) to the instrument.



Accessing the Online Help

Press **<Help>** to access the Online Help. To close the help, just press **<Help>** again.

Use the **arrow navigation** and **<Select>** keys to navigate the Online Help. Also, you can press **<Menu>** to display a list of links to the main Online Help sections.

When you next use the Online Help it will display the same page as when you last used it.

What is in the Online Help?

The Online Help is divided into sections to help you quickly find the information you want. Press **<Home>** to access the Home page.

Getting Started - Contains an instrument tour, details of how to use the graphical user interface and the Online Help, plus safety information and measurement tutorials.

Instrument Setup and Use - Explains how to set up the instrument, recall stored settings, make measurements and view results. There is an Instrument Setup and Use section for each network that the instrument can test (e.g. SDH, SONET).

Instrument Details - Contains supplementary product information. It includes information on:







- **System Features** - available options, manufacturing data, setting time and date, using the keyboard lock, printing results, file management and creating/storing your own help files
- **Technical Support** - maintenance, instrument reboot information
- **Frequently Asked Questions**

Telecoms Concepts - A reference section including reference tables (payloads, signal rates, overhead bytes, etc.), a summary of the ITU Standards and information on applications.

Index - Contains a list of all features and procedures.

Glossary - An comprehensive telecoms glossary.

Which Keys Do I Press?

	Press the <Help> key access the Online Help. Press it again to take you back to the instrument settings.
	Press this key to return to the Home page.
	Use the <Back> key to go back to the previous page. If you have used the <Back> key, then the <Fwd> key takes you forward to where you have just come from.
	Use these keys to scroll up or down through the displayed page.
	Press <Menu> to display a drop-down list of the main contents of the online help. Use the Arrow navigation keys to select a heading, then press <Select> .
	Use the Arrow Navigation keys to move between hypertext links within an Online Help page. Then press <Select> to jump to the chosen topic.

Accessing the Index

To find information quickly on a particular topic press **<Menu>** and select **Index** when in the Online Help.

Creating/Accessing Your Own Help Files

You can add your own help files to the instrument and access them through the Online Help system. This may be useful if you wish to store specific instructions to help users carry out routine procedures or help them with problem solving.

Creating Your Own Help Files

See the Online Help for information on how to create your own help files and download them to the instrument:

- 1 Press the **<Help>** to open the Online Help.
- 2 Press the **<Home>** key to open the Home page.
- 3 Select the option **User's Own Help Files**.

Accessing Your Own Help Files

To access your own help files installed on the instrument:

- 1 Press the **<Help>** key to open the Online Help.
- 2 Press the **<Menu>** key and select **Your Own Help**.
- 3 The names of your own help files will be displayed as a list of links. Choose a link and press **<Select>** to jump to the file.

Installation Manual

See the Installation manual for:

- information on how to install and connect the instrument
- safety information
- a product description

User Resources on the CD-ROM

Use the CD ROM with a PC. It contains training materials and support information, including:

- User documentation
 - User Guide
 - Quick Reference Guide
 - Remote Control manual
 - Installation manual
- Product/application notes
- Multimedia presentations including an instrument tour
- Links to the product website for technical specifications
- Telecommunications glossary
- Frequently asked questions

2 Getting Help



3 Quick Reference Tables

Smart Test	16
Transmitter Functions	17
Receiver Functions	19
Results	20
Test Functions	22
Overhead Monitor	23
Overhead Setup	24
System Functions	25
Print Control	27

Only the main selections are listed here. Make your selection, then press the **<Select>** button on the instrument's front panel.

The Smart Test functions are listed first. Smart Test is a unique and powerful feature allowing quick access to commonly-used setup pages, and to the jitter, wander and SignalWizard applications.

Use the front panel **<Smart Test>** and **<Print Control>** keys for fast selection of Smart Test and Print Control functions. Use the **<Menu>** key to access all other functions.

For jitter and wander setup, see "Test Functions" on page 22. For jitter transfer and jitter/wander tolerance measurements, see "Smart Test" on page 16. For GFP/LAPS setup, see "Transmitter Functions" on page 17 and "Receiver Functions" on page 19.



Smart Test

You can use the front panel **<Smart Test>** button to quickly select one of the following:

Function – Using Smart Test	Path
SignalWizard	Press <Smart Test> , choose SignalWizard then press <Select> .
Using Smart Test shortcuts to frequently-used features	Press <Smart Test> , choose Shortcuts . Select an item from the list and press <Select> .
Jitter/Wander Tolerance	Press <Smart Test> , choose Jitter/Wander Tolerance then press <Select> .
Jitter Transfer	Press <Smart Test> , choose Jitter Transfer then press <Select> .
Stop Application	Press <Smart Test> , choose Stop Application then press <Select> .
Reset Instrument to default settings	Press <Smart Test> , choose Reset Instrument then press <Select> .

Transmitter Functions

Function – Transmitter Interface	Path
Setting Tx signal rate, interface, code, operating level	Press <Menu>, choose Tx/Rx > Transmitter Settings > Physical then press <Select>.
Setting Tx OTN top level	Press <Menu>, choose Tx/Rx > Transmitter Settings > OTN then press <Select>.
Setting SDH Tx mapping	Press <Menu>, choose Tx/Rx > Transmitter Settings > SDH then press <Select>.
Setting SONET Tx mapping	Press <Menu>, choose Tx/Rx > Transmitter Settings > SONET then press <Select>.
Setting Tx GFP/LAPS framing protocol	Press <Menu>, choose Tx/Rx > Transmitter Settings > GFP/LAPS then press <Select>.
Generating Tx Ethernet payloads	Press <Menu>, choose Tx/Rx > Transmitter Settings > Ethernet then press <Select>.
Setting Tx test pattern	Press <Menu>, choose Tx/Rx > Transmitter Settings > Pattern then press <Select>.
Setting Tandem Connection Monitoring (SDH only)	Press <Menu>, choose Tx/Rx > Transmitter Settings > SDH then press <Select>.
Setting Thru Mode	Press <Menu>, choose Tx/Rx > Thru Mode then press <Select>.

3 Quick Reference Tables

Function – Transmitter Interface	Path
Coupling Transmit and Receive settings	Press <Menu>, choose Tx/Rx > Coupling then press <Select>.
Recall or Save instrument configuration	Press <Menu>, choose System > Stored Settings then press <Select>.

Receiver Functions

Function – Receiver Interface	Path
Setting Rx signal rate, interface, code, operating level	Press <Menu>, choose Tx/Rx > Receiver Settings > Physical then press <Select>.
Setting Rx OTN top level	Press <Menu>, choose Tx/Rx > Receiver Settings > OTN then press <Select>.
Setting SDH Rx mapping	Press <Menu>, choose Tx/Rx > Receiver Settings > SDH then press <Select>.
Setting SONET Rx mapping	Press <Menu>, choose Tx/Rx > Receiver Settings > SONET then press <Select>.
Setting Rx GFP/LAPS framing protocol	Press <Menu>, choose Tx/Rx > Receiver Settings > GFP/LAPS then press <Select>.
Setting up Rx Ethernet payloads	Press <Menu>, choose Tx/Rx > Receiver Settings > Ethernet then press <Select>.
Setting Rx test pattern	Press <Menu>, choose Tx/Rx > Receiver Settings > Pattern then press <Select>.
Setting TCM (SDH only)	Press <Menu>, choose Tx/Rx > Receiver Settings > SDH then press <Select>.
Coupling Transmit and Receive settings	Press <Menu>, choose Tx/Rx > Coupling then press <Select>.
Recall or Save instrument configuration	Press <Menu>, choose System > Stored Settings then press <Select>.

Results

Function – Results and Measurement Timing/Logging	Path
View Trouble Scan results	Press <Menu>, choose Results > Trouble Scan then press <Select>.
View OTN (for example) Alarm Seconds results	Press <Menu>, choose Results > Errors and Alarms > OTN then press <Select>. Select the Alarms Seconds tab.
View Measurement OTN (for example) Errors results	Press <Menu>, choose Results > Errors and Alarms > OTN then press <Select>. Select the Errors tab.
View Jitter/Wander measurement results	Press <Menu>, choose Results > Jitter/Wander then press <Select>.
Measure Performance Analysis	Press <Menu>, choose Results > Performance Analysis then press <Select>.
View OPU offset results	Press <Menu>, choose Results > Network Measurements > OPU Offset then press <Select>.
Measure AU/SPE Pointer activity	Press <Menu>, choose Results > Network Measurements > Pointers then press <Select>.
View GFP/LAPS results overview	Press <Menu>, choose Results > Errors and Alarms > GFP/LAPS then press <Select>. Select the Errors tab.

Function – Results and Measurement Timing/Logging	Path
View GFP/LAPS results details	Press <Menu>, choose Results > Network Measurements > GFP/LAPS then press <Select>. Select the Detail tab.
View Ethernet results overview	Press <Menu>, choose Results > Error and Alarms > Ethernet then press <Select>. Select the Errors tab.
View Ethernet results details	Press <Menu>, choose Results > Network Measurements > Ethernet then press <Select>. Select the Detail tab.
View Service Disruption results	Press <Menu>, choose Results > Network Measurements > Service Disruption then press <Select>.
View Optical Power results	Press <Menu>, choose Results > Signal Quality > Optical Power then press <Select>.
View Frequency results	Press <Menu>, choose Results > Signal Quality > Frequency Meas then press <Select>.
View Measurement Record System	Press <Menu>, choose Measurement Record > Graph Manager then press <Select>.
Setting Measurement Timing	Press <Menu>, choose Results > Measurement Setup > Timing then press <Select>.
Setting up Measurement Logging (logging settings, interval reports)	Press <Menu>, choose Results > Measurement Setup > Logging then press <Select>.

Test Functions

Function – Test Functions	Path
Adding Errors and Alarms to the transmit signal	Press <Menu>, choose Test Functions > Errors and Alarms then press <Select>.
Generating/monitoring Jitter/Wander	Press <Menu>, choose Test Functions > Jitter/Wander then press <Select>.
Add Runt/Jumbo Frames	Press <Menu>, choose Test Functions > Runt/Jumbo Add then press <Select>.
Adding Frequency Offset to the transmitted line signal	Press <Menu>, choose Test Functions > Frequency Offset then press <Select>.
Adding Pointer Adjustments	Press <Menu>, choose Test Functions > Pointer Adjustment then press <Select>.
Inserting or dropping the Data Communications Channel/General Communications Channel	Press <Menu>, choose Test Functions > DCC/GCC Drop/Insert then press <Select>.
Setting Transmit/Receive Triggers	Press <Menu>, choose Test Functions > Trigger Output then press <Select>.
Perform instrument Self Test	Press <Menu>, choose System > Self Test then press <Select>.
Switch off Test Functions	Press <Menu>, choose Test Functions > Switch Off then press <Select>.

Overhead Monitor

Function – Selecting Receiver Overhead Monitor	Path
Using Rx Overhead Monitor Trace Messages	Press <Menu>, choose Overhead Monitor > Trace Messages then press <Select>.
Using Rx Overhead Labels (Signal Labels, Sync Status)	Press <Menu>, choose Overhead Monitor > Labels then press <Select>.
Using Rx Overhead APS Messages	Press <Menu>, choose Overhead Monitor > APS Messages then press <Select>.
Using Rx Overhead Bytes	Press <Menu>, choose Overhead Monitor > Byte Monitor then press <Select>.
To Capture an Overhead Sequence	Press <Menu>, choose Overhead Monitor > Sequence Capture then press <Select>. Select the Sequence Capture tab.
To Capture Data (OTN frames, SONET/SDH Overheads)	Press <Menu>, choose Overhead Monitor > Data Capture then press <Select>.

Overhead Setup

Function – Selecting Transmitter Overhead	Path
Setting Tx Overhead Trace Messages	Press <Menu>, choose Overhead Setup > Trace Messages then press <Select>.
Setting Tx Overhead Labels (Signal Labels, Sync Status)	Press <Menu>, choose Overhead Setup > Labels then press <Select>.
Setting Tx Overhead APS Messages	Press <Menu>, choose Overhead Setup > APS Messages then press <Select>.
Setting Tx Overhead Bytes	Press <Menu>, choose Overhead Setup > Byte Setup then press <Select>.
Setting Tx Overhead Sequences	Press <Menu>, choose Overhead Setup > Sequence Generation then press <Select>.
Restore Byte Default values	Press <Menu>, choose Overhead Setup > Restore Defaults then press <Select>.

System Functions

Function – Remote Control, Date/Time Settings, Preferences, Calibration	Path
View System Options, Software Revision	Press <Menu>, choose System > Options then press <Select>.
System Preferences: MS-REI/REI-L result monitor selection MS-AIS/AIS-L alarm monitor selection G.826 collect ES, SES, BBE enable Enhanced RDI enable Select M0, M1 byte usage Beep on Error audio control Save System Preferences settings as default	Press <Menu>, choose System > Preferences then press <Select>.
Set up remote operation via RS 232, GPIB or LAN	Press <Menu>, choose System > Remote Control then press <Select>.
Setting Time and Date	Press <Menu>, choose System > Time and Date then press <Select>.
Calibrate instrument	Press <Menu>, choose System > Calibration then press <Select>.

System Functions – File Manager

Function – File Manager	Path
Copy/delete logging files to/from the floppy disk drive	Press <Menu>, choose System > File Manager then press <Select>. Select the Logging tab.
Copy/download Screen Dumps to/from the floppy disk drive	Press <Menu>, choose System > File Manager then press <Select>. Select the Screen Dump tab.
Copy/download Stored Settings to/from the floppy disk drive	Press <Menu>, choose System > File Manager then press <Select>. Select the Settings tab.
Copy/download your own User Help files to/from the floppy disk.	Press <Menu>, choose System > File Manager then press <Select>. Select the User Help tab.

Print Control

Use the front panel **<Print Control>** button to select one of the following:

Function – Print Control	Path
Copy a snapshot of the logging results to a Printer/File	Press <Menu> , choose Results > Measurement Setup > Logging then press <Select> .
Copy a screen dump of current window to a file or Printer	Press <Print Control> .

3 Quick Reference Tables

Index

C

- CD-ROM resources, 13
- Conventions used in this guide, 4

D

- Description, product, 8

E

- Enabling Tandem Connection Monitoring (TCM)
 - receiver setup, 19
 - transmitter setup, 17

I

- Installation manual, 13

O

- Online Help
 - accessing, 10
 - contents, 10
 - index, 11
 - own help files, 12

P

- Product notes (on CD-ROM), 13

R

- Reference tables
 - accessing instrument features, 15
- Remote Control manual (on CD-ROM), 13

T

- Training resources (on CD-ROM), 13


U

- User Guide (on CD-ROM), 13

Notes:

Notes:

Navigating the Graphical User Interface

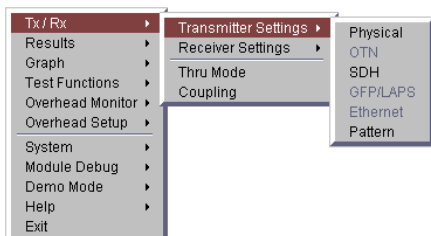

Using the Instrument:

1. Press the **<Menu>** key.
2. Use the Arrows and **<Select>** key to choose a title from the menu.
3. Use the Arrows and **<Select>** key to set up the instrument, by moving around the folders, drop-down boxes, text/numeric-entry boxes and dialog boxes.

Using an External Mouse/Keyboard:

1. Connect a mouse and keyboard.
2. Switch on the instrument.
3. Right-click to display the menu.
4. Choose a GUI page title and set up the instrument using the mouse. To enter data, use the external keyboard instead of the instrument keypad.

Front Panel/Graphical User Interface (GUI)

Online Help:
Press **<Help>** for help using the GUI and front panel keys.

Active Window:
Press **<Window>** to change the active window.

Context Sensitive Help: Displays information about the active part of the GUI.

Status and Alarm LEDs,
<Show More> and History **<Reset>** Keys

Function Keys:
<Run/Stop>,
<Smart Test>,
<Single Error> and
<Help>

Navigation Keys:
Arrows, **<Select>**,
<Menu>, **<Window>**
and **<Cancel>**

Keypad:
For numeric/text entry
and navigating the
Online Help.


<Print Control> Key



Summary Diagram:
Displays current settings,
test function indicators and
elapsed measurement time.

Instrument Status Line

Connector Panel

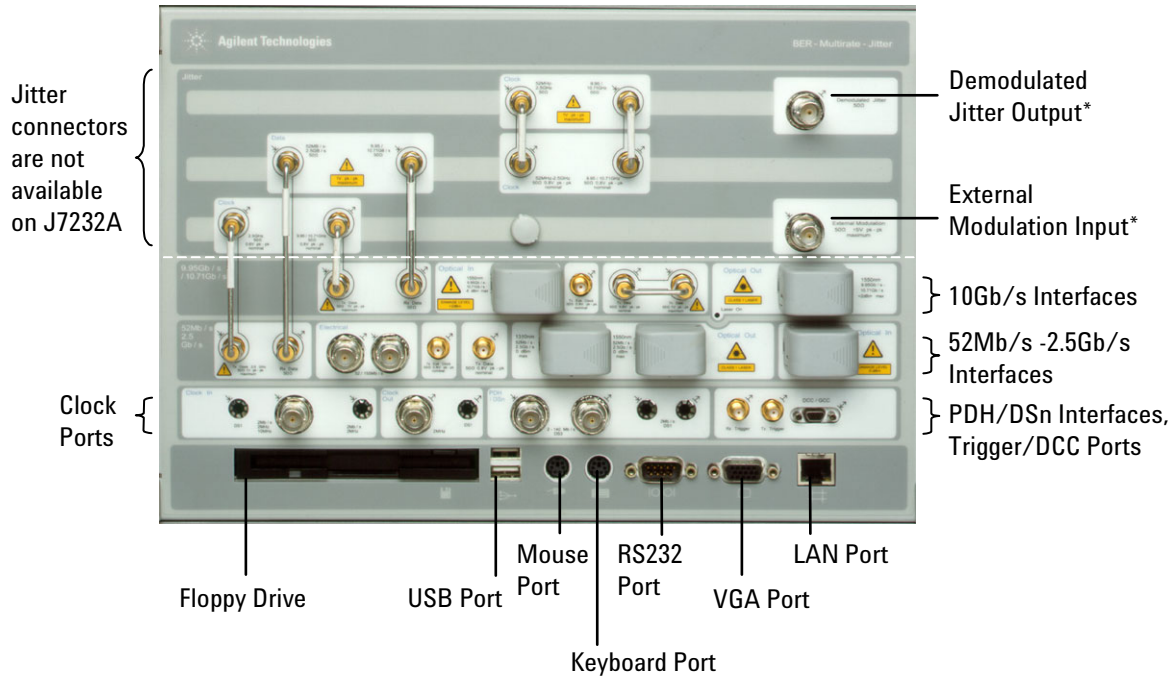

*J7231B connector panel shown. Jitter connectors not available on J7232A.

Sources of Help

Online Help:

Includes information on setting up the instrument, adding your own help files to the instrument, plus a technology reference section.

To access help information for new users, including the measurement tutorials:

1. Press the **<Help>** key.
2. Press the **<Home>** key (top left key on the keypad).
3. Select 'Getting Started' using the arrow keys and **<Select>** key.
4. Use the keys on the top row of the keypad to navigate the Online Help.

CD-ROM:

Includes all user documentation, product notes, frequently-asked questions, a glossary and multimedia training presentations.

Installation Manual:

Includes information on connecting the instrument, plus safety information.

In this book:

- * Overview of user interface
- * Quick Reference Tables for selection of main instrument functions.
- * Sources of detailed information
- * Introduction to the comprehensive Online Help Facility.

Printed in U.K. 08/03
J7230-90053



Agilent Technologies