



# Agilent 75000 SERIES B

## E1300B/E1301B Mainframe E1306A Command Module Memory Module

---

### Installation Note



Copyright© Agilent Technologies, Inc., 1995, 2006



E1300-90027  
E0206



---

## Certification

*Agilent Technologies certifies that this product met its published specifications at the time of shipment from the factory. Agilent Technologies further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology (formerly National Bureau of Standards), to the extent allowed by that organization's calibration facility, and to the calibration facilities of other International Standards Organization members.*

---

## Warranty

This Agilent Technologies product is warranted against defects in materials and workmanship for a period of one year from date of shipment. Duration and conditions of warranty for this product may be superseded when the product is integrated into (becomes a part of) other Agilent products. During the warranty period, Agilent Technologies will, at its option, either repair or replace products which prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by Agilent Technologies. Buyer shall pre-pay shipping charges to Agilent and Agilent shall pay shipping charges to return the product to Buyer. However, Buyer shall pay all shipping charges, duties, and taxes for products returned to Agilent from another country.

Agilent warrants that its software and firmware designated by Agilent for use with a product will execute its programming instructions when properly installed on that product. Agilent does not warrant that the operation of the product, or software, or firmware will be uninterrupted or error free.

## Limitation Of Warranty

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by Buyer, Buyer-supplied products or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

The design and implementation of any circuit on this product is the sole responsibility of the Buyer. Agilent does not warrant the Buyer's circuitry or malfunctions of Agilent products that result from the Buyer's circuitry. In addition, Agilent does not warrant any damage that occurs as a result of the Buyer's circuit or any defects that result from Buyer-supplied products.

NO OTHER WARRANTY IS EXPRESSED OR IMPLIED. Agilent SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

## Exclusive Remedies

THE REMEDIES PROVIDED HEREIN ARE BUYER'S SOLE AND EXCLUSIVE REMEDIES. Agilent SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER BASED ON CONTRACT, TORT, OR ANY OTHER LEGAL THEORY.

---

## Notice

The information contained in this document is subject to change without notice. Agilent Technologies MAKES NO WARRANTY OF ANY KIND WITH REGARD TO THIS MATERIAL, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. Agilent shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance or use of this material. This document contains proprietary information which is protected by copyright. All rights are reserved. No part of this document may be photocopied, reproduced, or translated to another language without the prior written consent of Agilent Technologies, Inc. Agilent assumes no responsibility for the use or reliability of its software on equipment that is not furnished by Agilent.

---

## U.S. Government Restricted Rights

The Software and Documentation have been developed entirely at private expense. They are delivered and licensed as "commercial computer software" as defined in DFARS 252.227-7013 (Oct 1988), DFARS 252.211-7015 (May 1991) or DFARS 252.227-7014 (Jun 1995), as a "commercial item" as defined in FAR 2.101(a), or as "Restricted computer software" as defined in FAR 52.227-19 (Jun 1987)(or any equivalent agency regulation or contract clause), whichever is applicable. You have only those rights provided for such Software and Documentation by the applicable FAR or DFARS clause or the Agilent standard software agreement for the product involved.

---

Agilent E1300B/E1301B Mainframes and E1306A Command Module  
Memory Module Installation Note  
Edition 2 Rev 2

Copyright © 1995-2006 Agilent Technologies, Inc. All Rights Reserved.

## Printing History

The Printing History shown below lists all Editions and Updates of this manual and the printing date(s). The first printing of the manual is Edition 1. The Edition number increments by 1 whenever the manual is revised. Updates, which are issued between Editions, contain replacement pages to correct the current Edition of the manual. Updates are numbered sequentially starting with Update 1. When a new Edition is created, it contains all the Update information for the previous Edition. Each new Edition or Update also includes a revised copy of this printing history page. Many product updates or revisions do not require manual changes and, conversely, manual corrections may be done without accompanying product changes. Therefore, do not expect a one-to-one correspondence between product updates and manual updates.

Edition 1 (Part Number E1300-90021) . . . . . September 1990  
Edition 2 (Part Number E1300-90027) . . . . . January 1995  
Edition 2 Rev 2 (Part Number E1300-90027) . . . . . February 2006

---


## Safety Symbols



Instruction manual symbol affixed to product. Indicates that the user must refer to the manual for specific **WARNING** or **CAUTION** information to avoid personal injury or damage to the product.



Indicates the field wiring terminal that must be connected to earth ground before operating the equipment—protects against electrical shock in case of fault.



Frame or chassis ground terminal—typically connects to the equipment's metal frame.



Alternating current (AC).



Direct current (DC).



Indicates hazardous voltages.

**WARNING**

Calls attention to a procedure, practice, or condition that could cause bodily injury or death.

**CAUTION**

Calls attention to a procedure, practice, or condition that could possibly cause damage to equipment or permanent loss of data.

---

## WARNINGS

**The following general safety precautions must be observed during all phases of operation, service, and repair of this product. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the product. Agilent Technologies assumes no liability for the customer's failure to comply with these requirements.**

**Ground the equipment:** For Safety Class 1 equipment (equipment having a protective earth terminal), an uninterruptible safety earth ground must be provided from the mains power source to the product input wiring terminals or supplied power cable.

**DO NOT operate the product in an explosive atmosphere or in the presence of flammable gases or fumes.**

For continued protection against fire, replace the line fuse(s) only with fuse(s) of the same voltage and current rating and type. DO NOT use repaired fuses or short-circuited fuse holders.

**Keep away from live circuits:** Operating personnel must not remove equipment covers or shields. Procedures involving the removal of covers or shields are for use by service-trained personnel only. Under certain conditions, dangerous voltages may exist even with the equipment switched off. To avoid dangerous electrical shock, DO NOT perform procedures involving cover or shield removal unless you are qualified to do so.

**DO NOT operate damaged equipment:** Whenever it is possible that the safety protection features built into this product have been impaired, either through physical damage, excessive moisture, or any other reason, REMOVE POWER and do not use the product until safe operation can be verified by service-trained personnel. If necessary, return the product to an Agilent Technologies Sales and Service Office for service and repair to ensure that safety features are maintained.

**DO NOT service or adjust alone:** Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

**DO NOT substitute parts or modify equipment:** Because of the danger of introducing additional hazards, do not install substitute parts or perform any unauthorized modification to the product. Return the product to an Agilent Technologies Sales and Service Office for service and repair to ensure that safety features are maintained.

# Chapter 1

## Installing Memory into an Agilent E1300B/E1301B Mainframe

---

### Description

You can install one or two memory modules onto the controller circuit board in the Agilent E1300B/E1301B Mainframe. Any combination of the 512kByte and 1MByte modules can be used to produce 512 k, 1 M, 1.5M or 2M of nonvolatile memory. The new memory will be used instead of (not in addition to) the standard 64k of built-in controller board memory.

### Warnings and Cautions

---

**WARNING**    **SHOCK HAZARD.** Only service-trained personnel who are aware of the hazards involved should install, remove, or configure the system. Before you perform any procedures in this guide, disconnect AC power and field wiring from the mainframe.

---

**Caution**     Do not install or remove modules with power applied to the mainframe. Doing so may damage the modules and the mainframe.

---

**Caution**     **STATIC ELECTRICITY.** Static electricity is a major cause of component failure. To prevent damage to the electrical components in the mainframe, plug-in modules, and memory modules, observe anti-static techniques whenever handling any of this equipment.

---

### Installation Kit


The following items comprise the memory module installation kit:

- #10 Torx®\* Key - 1 each
- #10 Torx® screws - 4 each
- Nonvolatile Memory Module - 1 each


\* Torx is a registered trademark of the Camcar Division of Textron Inc.

# Installation Procedure


## Step 1: Disconnect the mainframe's power.

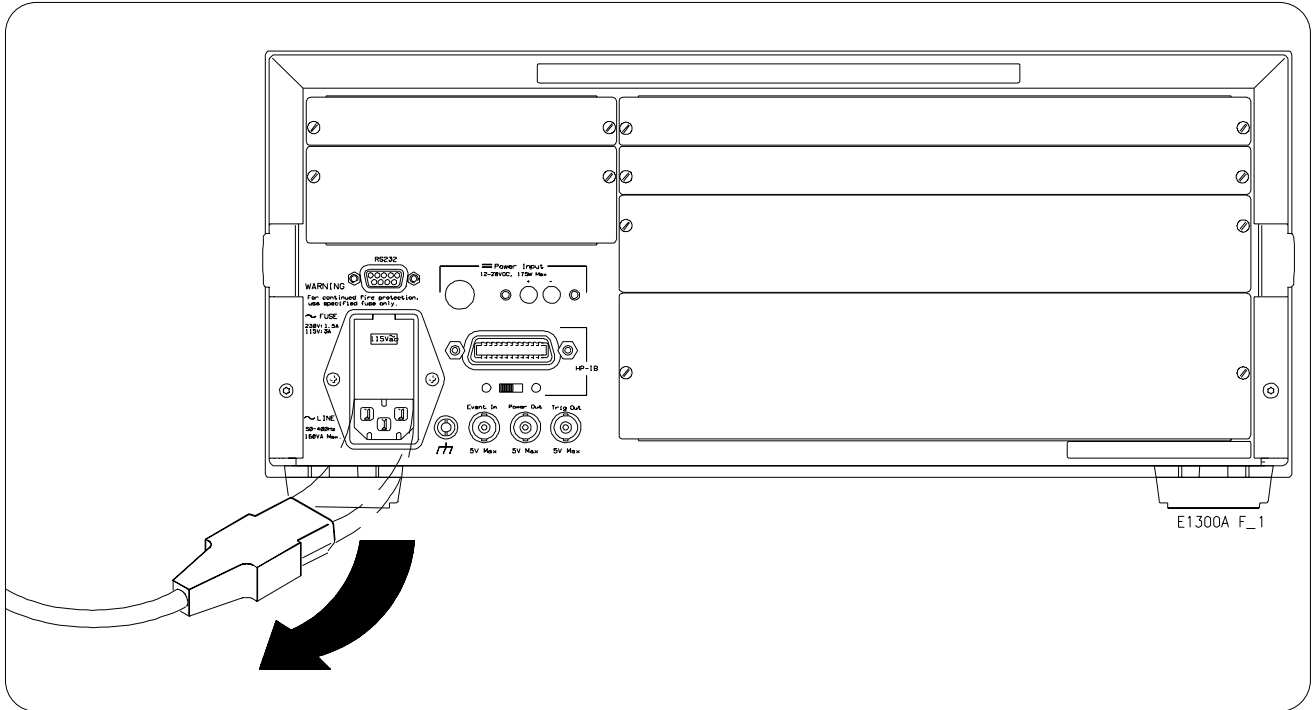

## Step 2: Remove the mainframe's side handles.

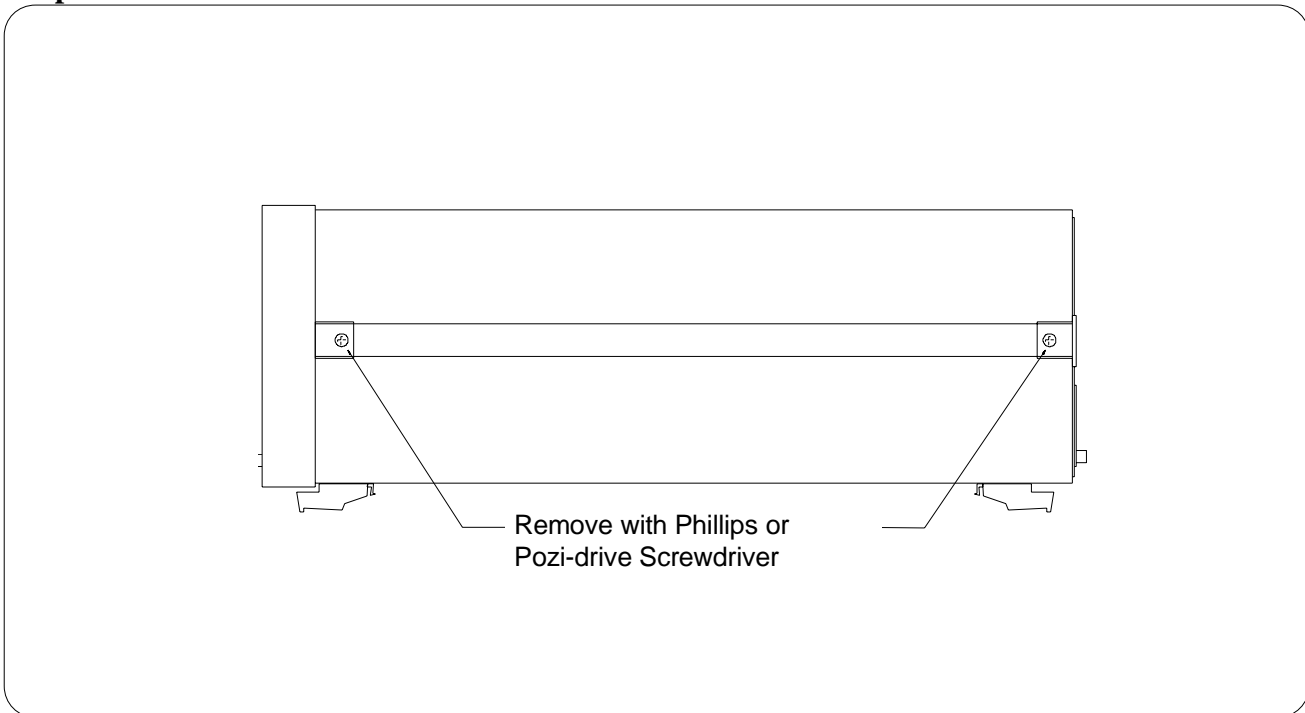


**Step 3: Remove the Torx® screws on the rear of the mainframe.**

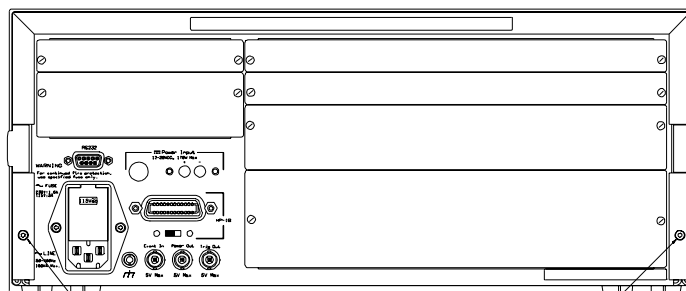


Remove with T10 Torx Key

**Step 4: Slide the top cover toward the rear, lift and remove the cover.**

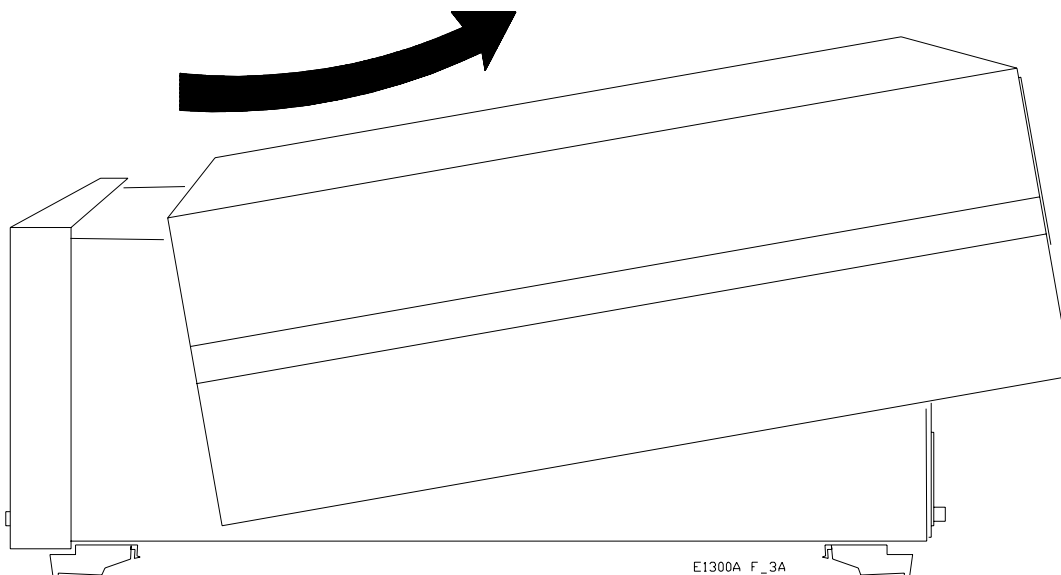


E1300A F\_3A

**Step 5: Remove the screw securing the support bracket. Lift the rear of the support bracket to disconnect it from the controller front support and remove the support bracket.**

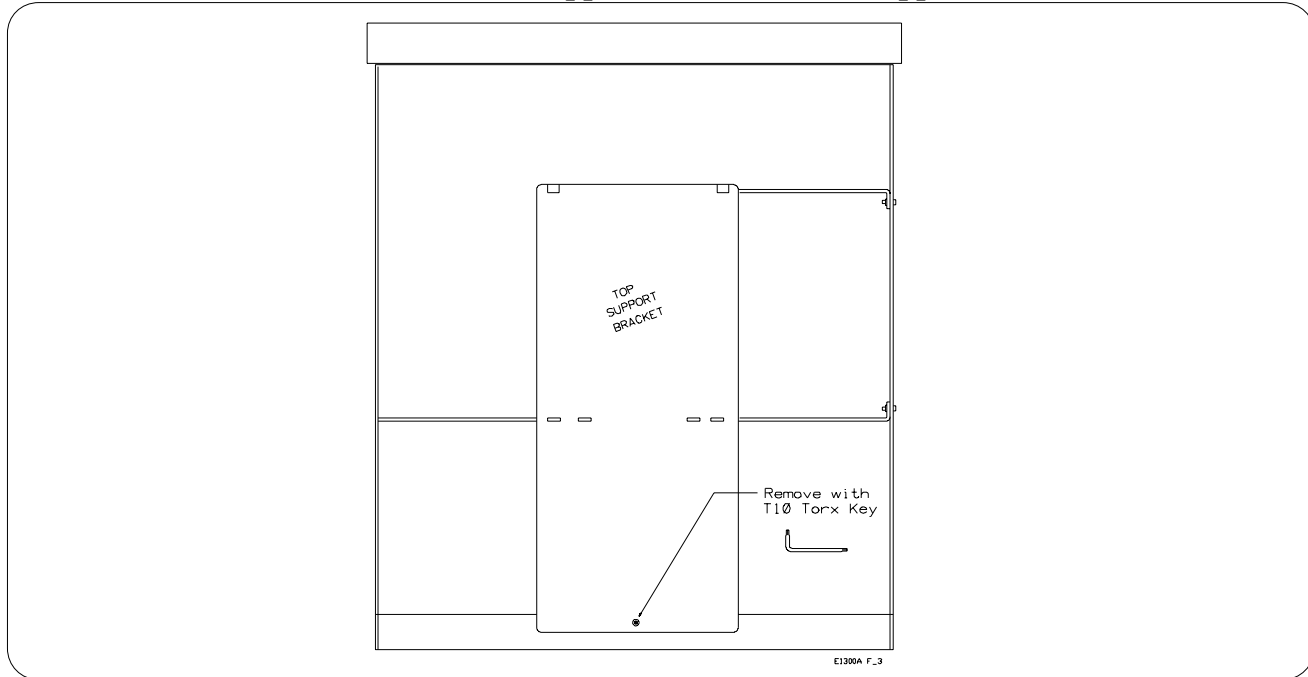


**Step 6: If you have an internal Agilent E1326 5 1/2 Digit Multimeter, disconnect the BNC cable, and remove the three Torx® screws.**

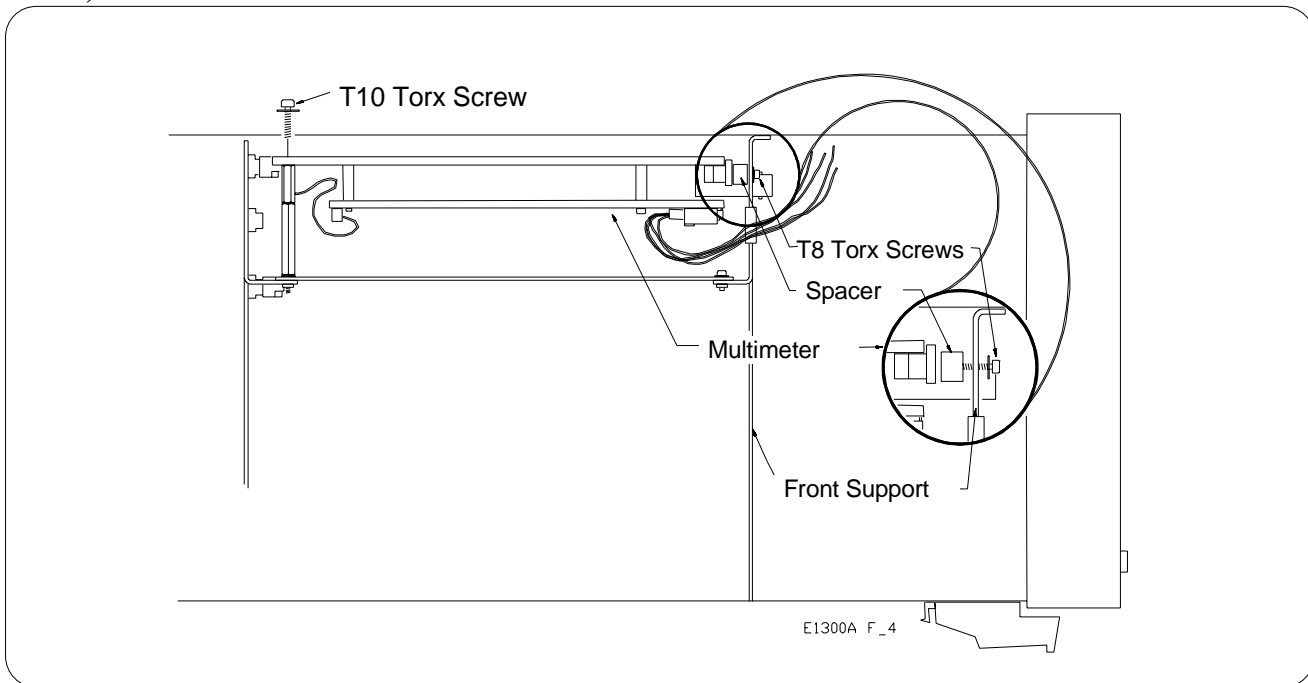





**Step 7: Remove the multimeter.**

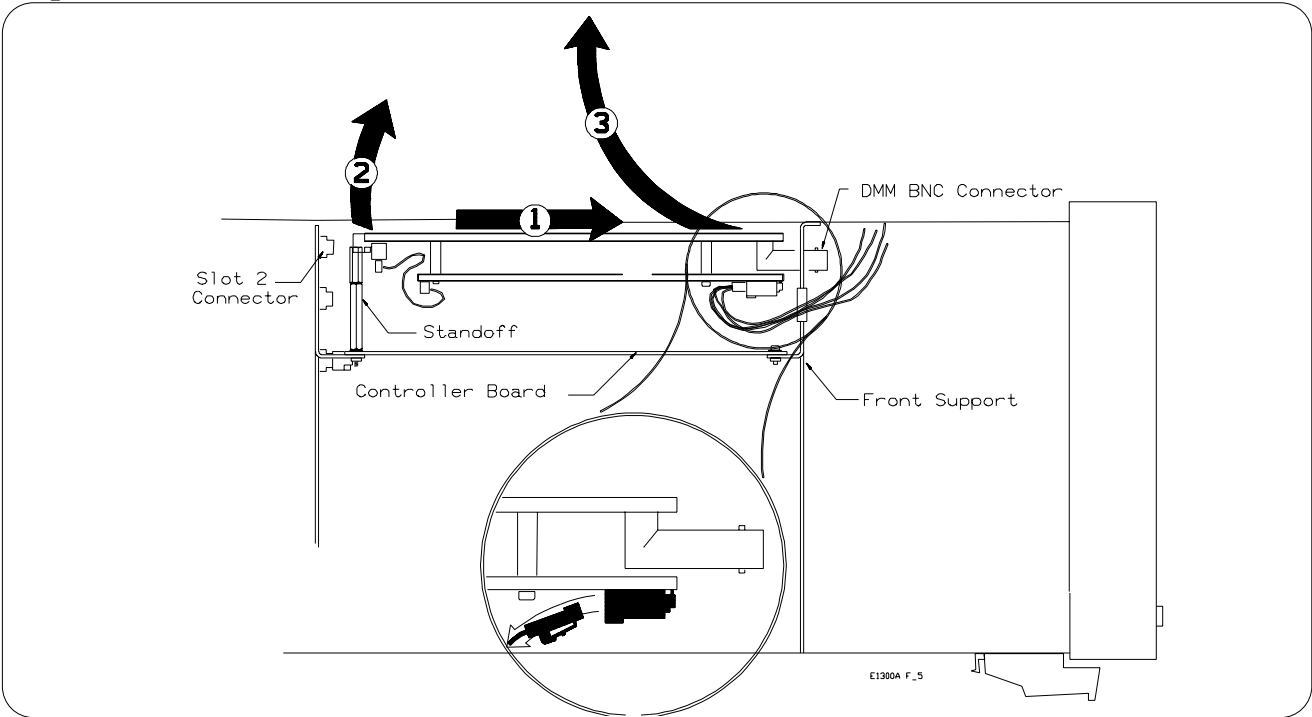


**Step 8: Remove the three T10 Torx® screws securing the controller board.**

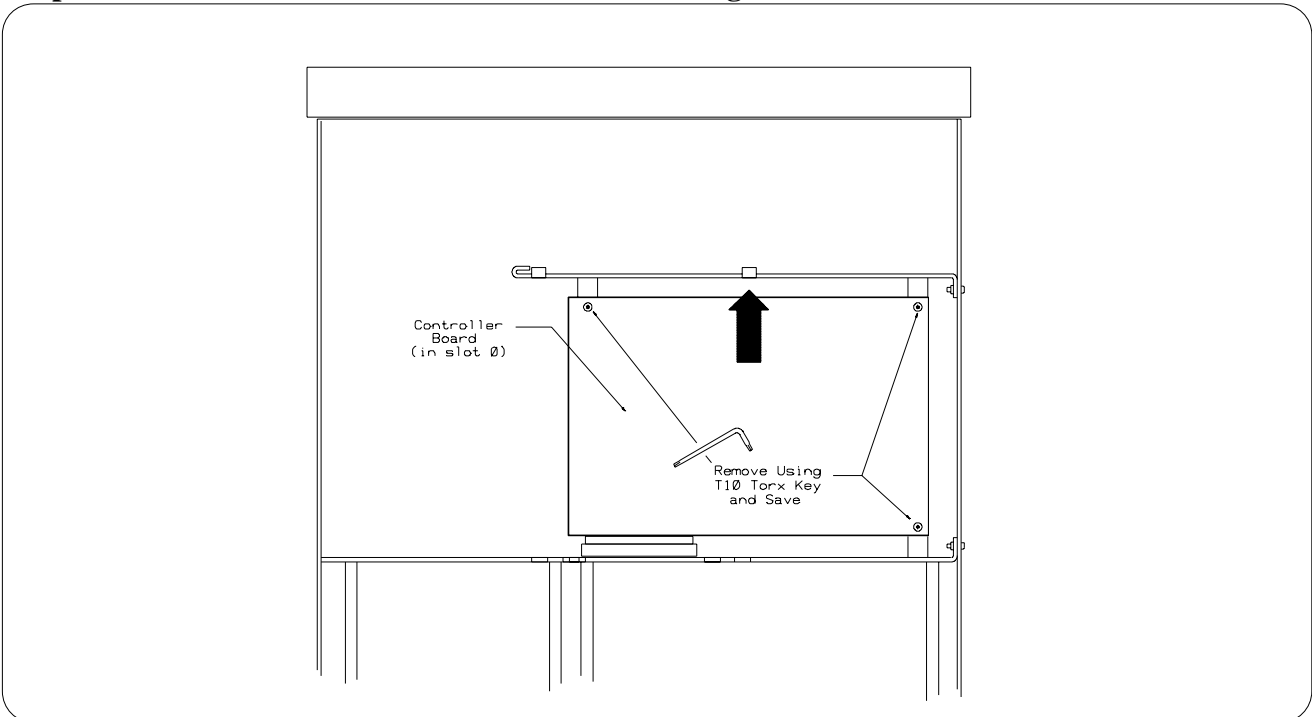

**Step 9: Remove the controller module's ribbon cable connector(s) (the E1300 has one ribbon cable, the E1301 has two cables). Push the controller module forward through the front controller support to disconnect it from the J1 connector. Remove the controller module.**

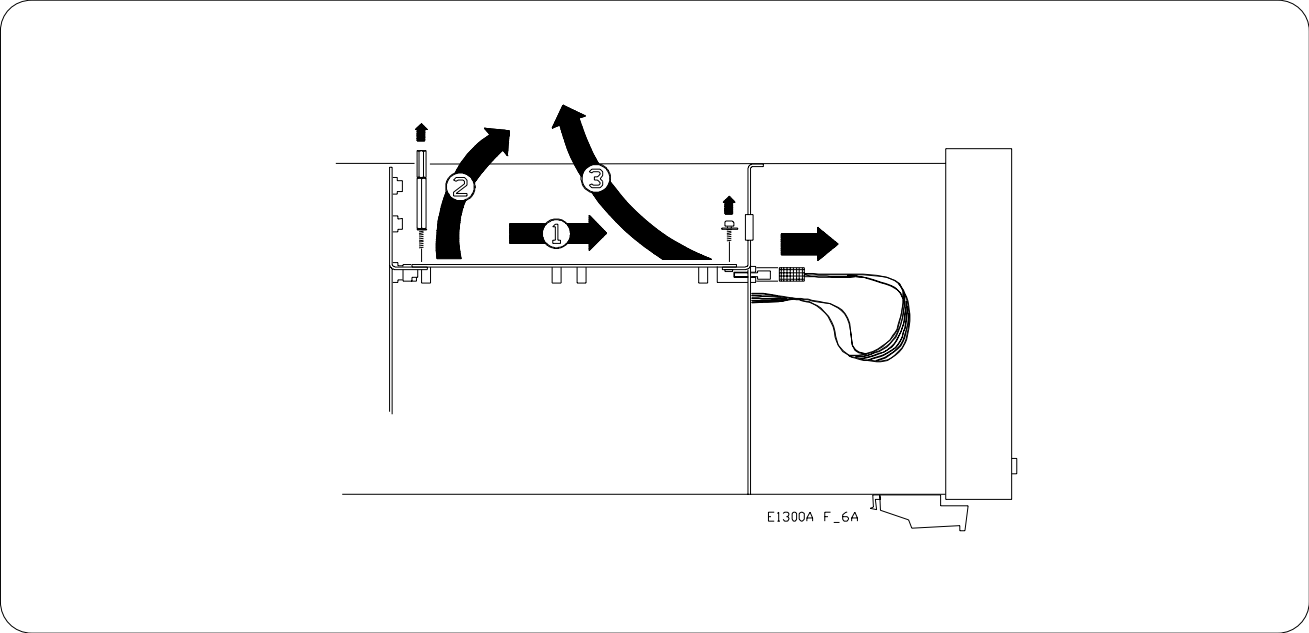

**Step 10: Set the memory module address switch(es) according to Table 1-1.**

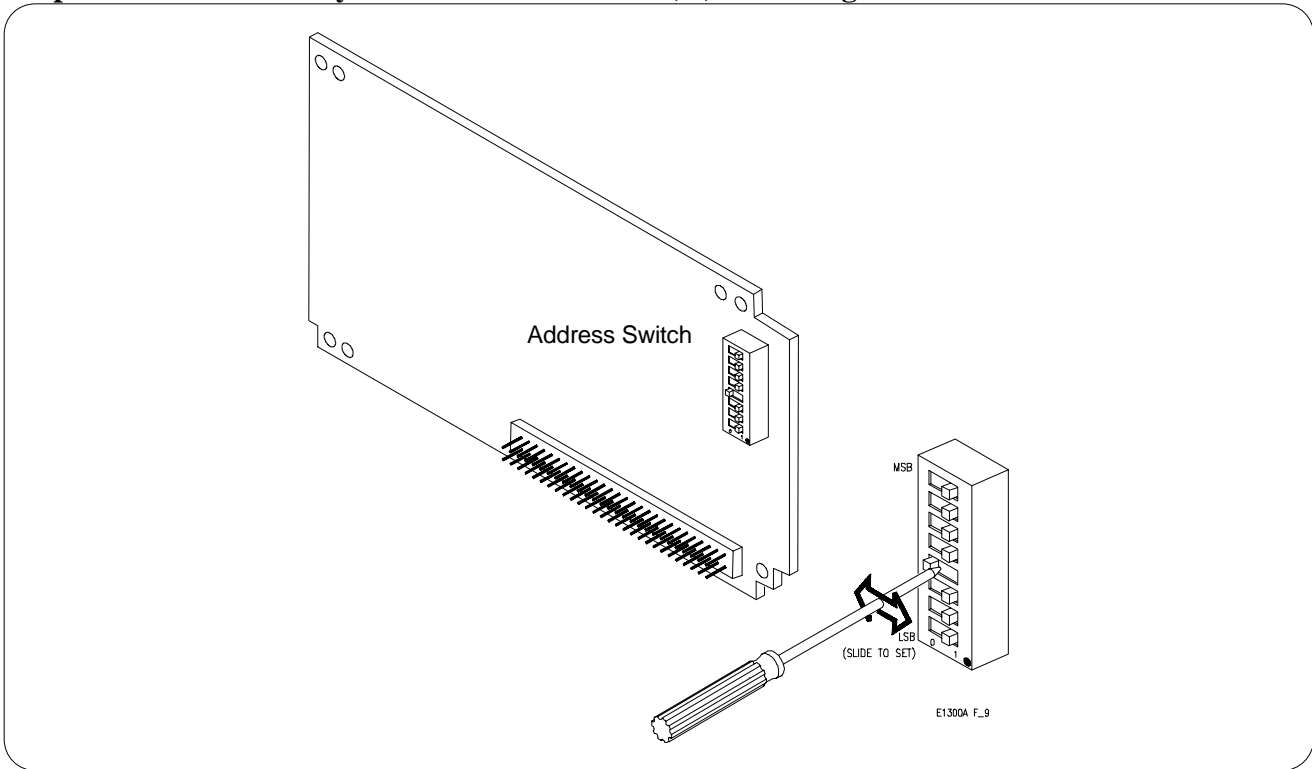


For example, in the figure above, the four Most Significant Bit (MSB) switches are shown in the "1" position, the next bit is shown in the "0" position. The three Least Significant bit switches (shown in the "1" position) are not used and may be in either the "1" or "0" position. Only the four Most Significant Bit address switches need to be set for the 1 MByte modules; or five Most Significant Bit address switches for the 512 kByte modules. Note: Ignore any numbering on the switch bank. Use the figure above to properly orient the address switch.

**Table 1-1. Memory Module Address Switch Settings**

<b>Module(s) being installed:</b>	<b>Set one module's address to:</b> ("x" signifies a "Don't Care" state)	<b>Set the other module's address to:</b> ("x" signifies a "Don't Care" state)
One 1 MByte Module	MSB 1 1 1 1 x x x x LSB	
Two 1MByte Modules	MSB 1 1 1 1 x x x x LSB	MSB 1 1 1 0 x x x x LSB
One 512 kByte Module	MSB 1 1 1 1 1 x x x LSB	
Two 512 kByte Modules	MSB 1 1 1 1 1 x x x LSB	MSB 1 1 1 1 0 x x x LSB
One 1 MByte Module and One 512 kByte Module	Set the <b>1MByte</b> module address to: MSB 1 1 1 1 x x x x LSB	Set the <b>512 kByte</b> module address to: MSB 1 1 1 0 1 x x x LSB

**Step 11: Install the memory module(s) and fasten with the Torx® screws provided.**

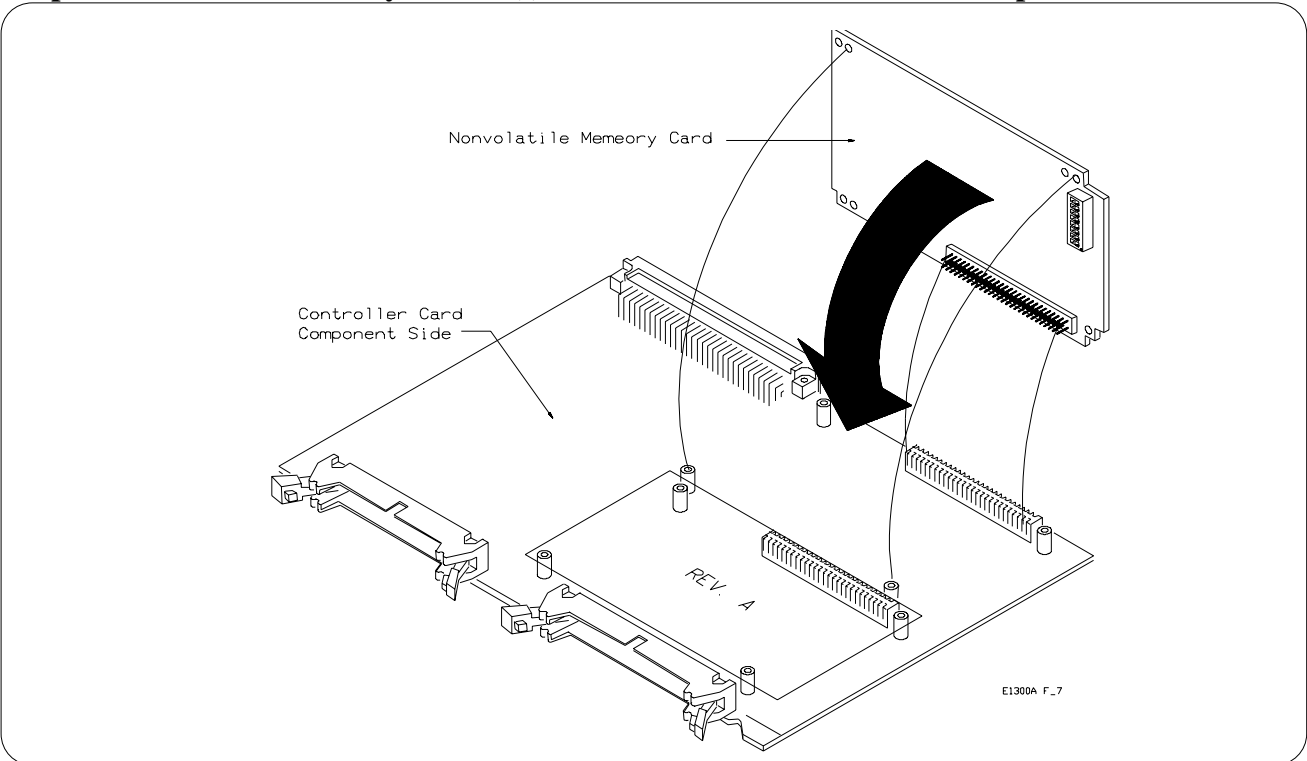

**Step 12: Reassemble the mainframe.**

## Chapter 2

# Installing Memory into an Agilent E1306A Command Module

---

## Description

You can install one or two 1MByte memory modules into an Agilent E1306A Command Module. The new memory will be used instead of (not in addition to) the standard 64k of built-in Command Module memory.

## Warnings and Cautions

---

**WARNING**    **SHOCK HAZARD.** Only service-trained personnel who are aware of the hazards involved should install, remove, or configure the system. Before you perform any procedures in this guide, disconnect AC power and field wiring from the mainframe.

---

**Caution**      **Do not install or remove modules with power applied to the mainframe. Doing so may damage the modules and the mainframe.**

---

**Caution**      **STATIC ELECTRICITY.** Static electricity is a major cause of component failure. To prevent damage to the electrical components in the mainframe, plug-in modules, and memory modules, observe anti-static techniques whenever handling any of this equipment.

---

## Installation Kit

The following items are included in the memory module installation kit:


- #10 Torx®\* Key - 1 each
- #10 Torx® screws - 4 each
- 1MByte Nonvolatile Memory Module - 1 each

\* Torx is a registered trademark of the Camcar Division of Textron Inc.


# Installation Procedure

**Step 1: If the Agilent E1306A Command Module is installed in a mainframe, disconnect power to the mainframe and remove the Command Module.**

**Step 2: Remove the Command Module's shield.**

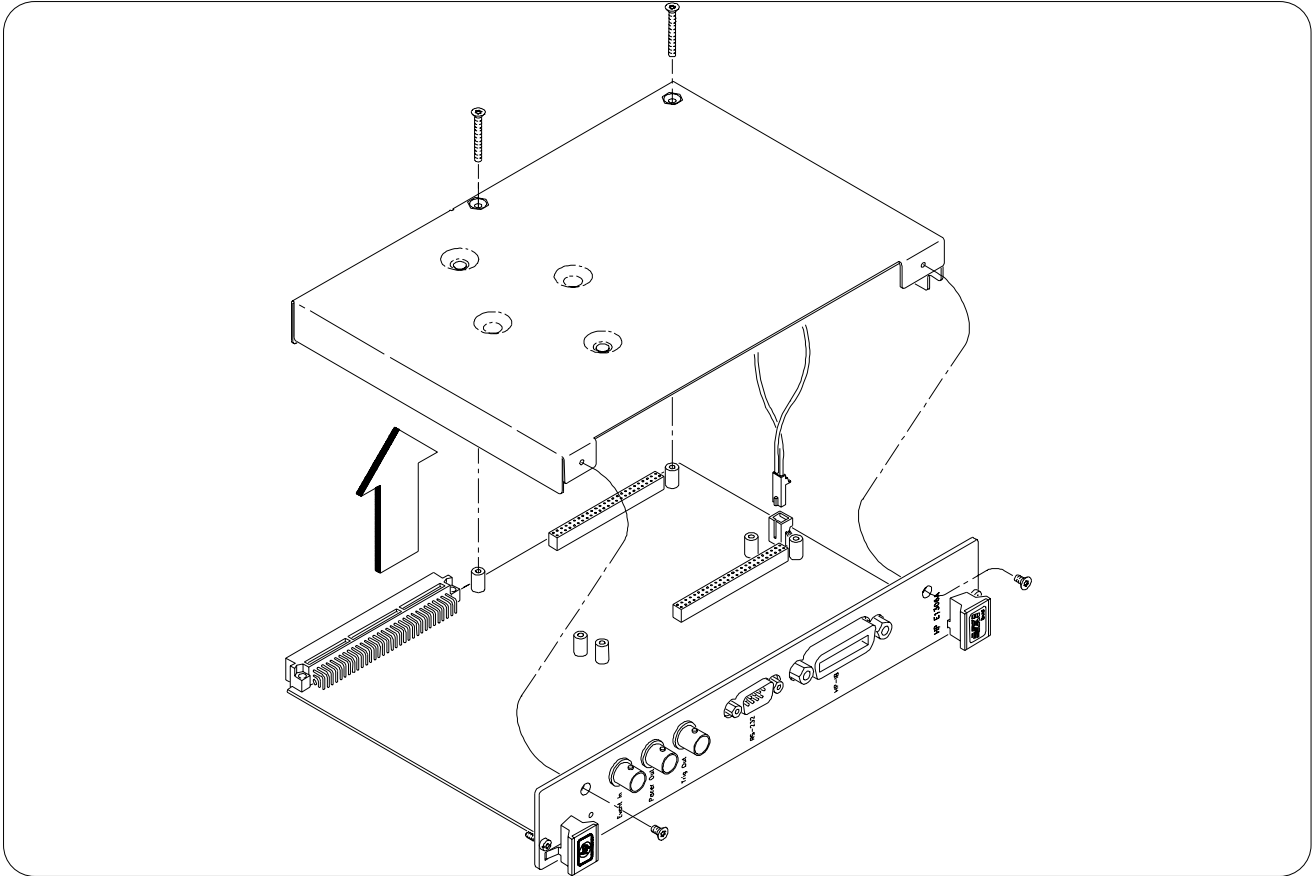

**Step 3: Set the memory module address switch(es) according to Table 2-1.**

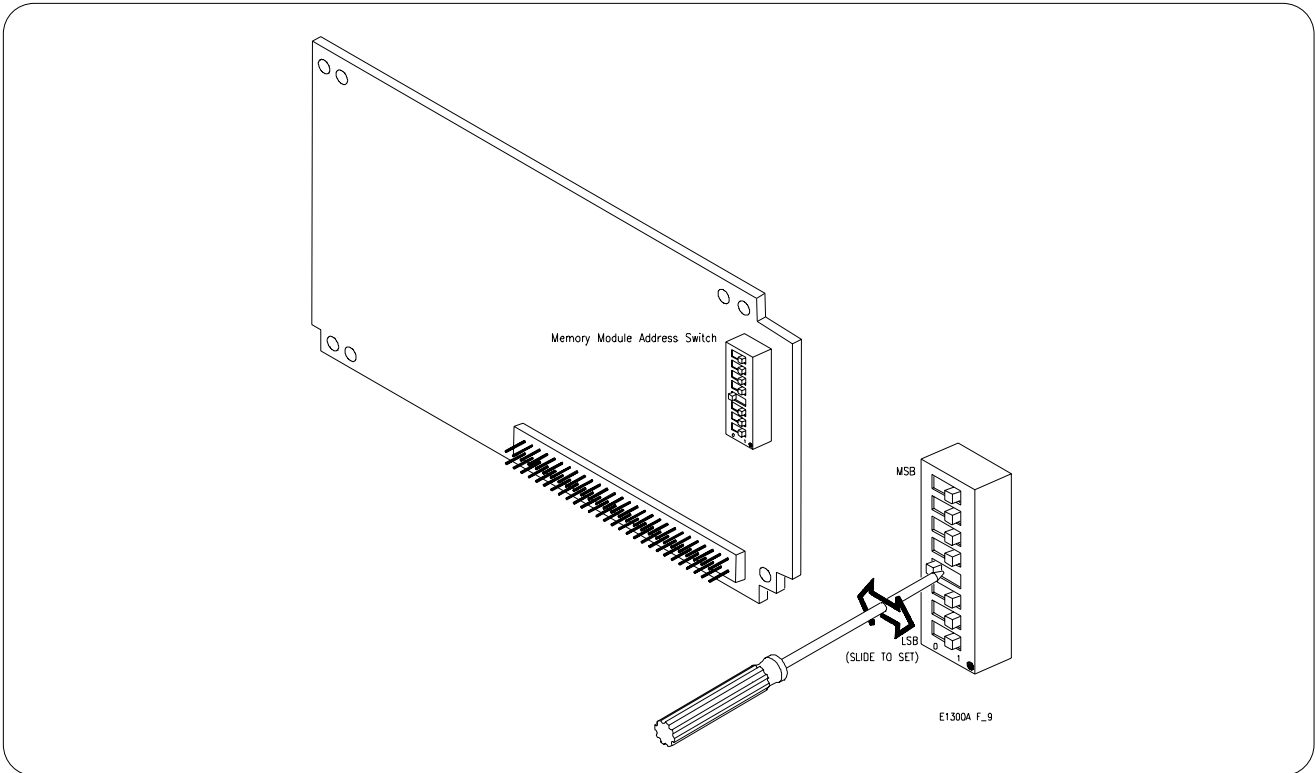


For example, in the figure above, the four Most Significant Bit (MSB) switches are shown in the "1" position, the next bit is shown in the "0" position. The three Least Significant bit switches (shown in the "1" position) are not used and may be in either the "1" or "0" position. Only the four Most Significant Bit address switches need to be set for the 1 MByte modules; or five Most Significant Bit address switches for the 512 kByte modules. Note: Ignore any numbering on the switch bank. Use the figure above to properly orient the address switch.

**Table 2-1. Memory Module Address Switch Settings**


<b>Module(s) being installed:</b>	<b>Set one module's address to:</b>	<b>Set the other module's address to:</b>
One 1 MByte Module	MSB 1 1 1 1 x x x x LSB	
Two 1MByte Modules	MSB 1 1 1 1 x x x x LSB	MSB 1 1 1 0 x x x x LSB

("x" signifies a "Don't Care" state)

**Step 4: Install the memory module and fasten with two Torx® screws.**

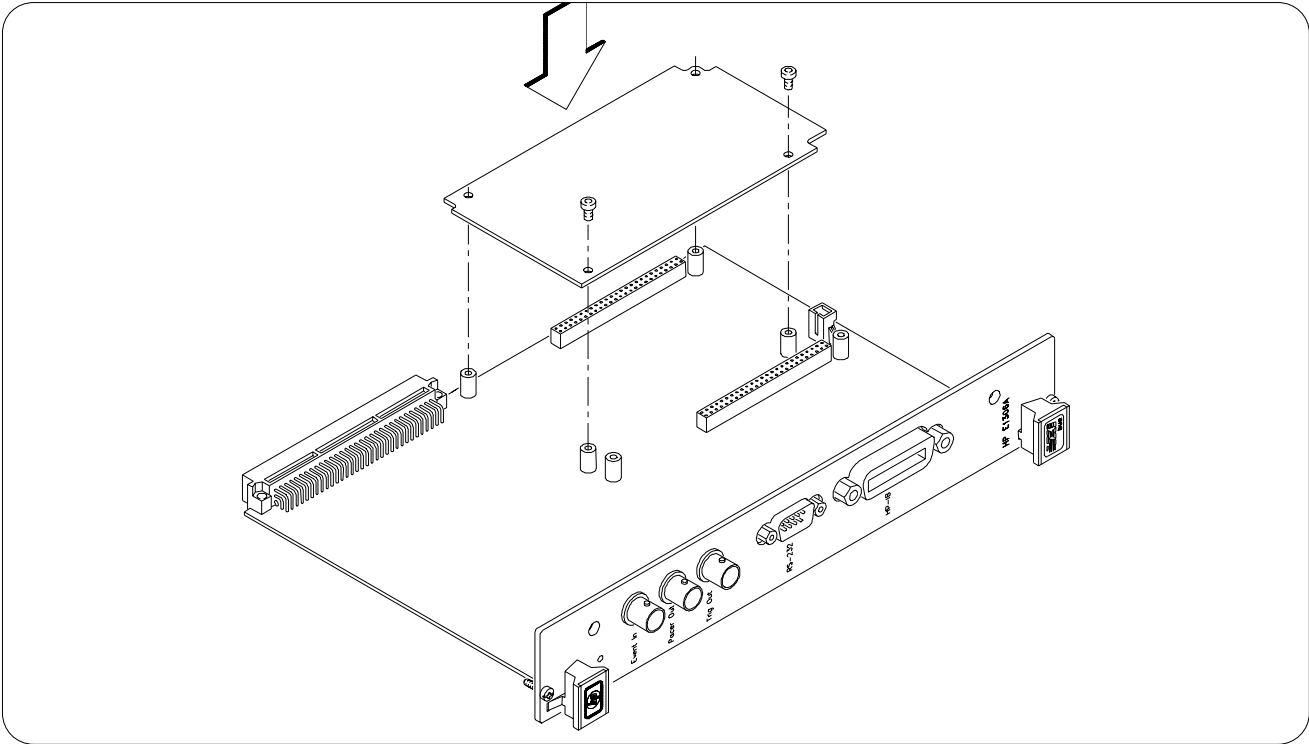

**Step 5: (Optional) Install second memory module and fasten with four Torx® screws.**

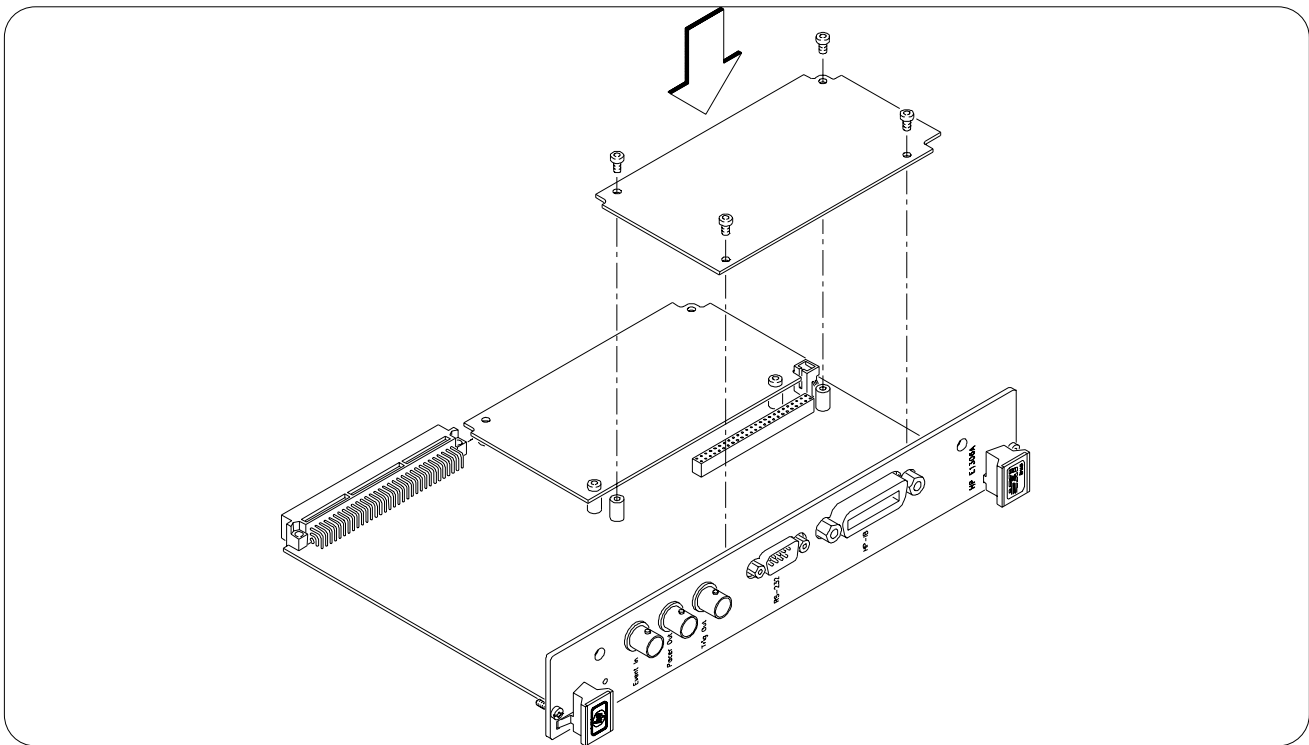

**Step 5: Reassemble the Command Module.**