Agilent 75000 Series B



Agilent E1351A/52A/53A/57A/58A FET Multiplexers

Service Manual

Enclosed is the Service Manual for the Agilent E1351A/52A/53A/57A/58A FET Multiplexers. Insert this manual, along with any other VXIbus manuals that you have, into the binder that came with your Agilent Mainframe.





Manual Part Number: E1351-90011 Printed in Malaysia E0606

Certification

Agilent Technologies certifies that this product met its published specifications at the time of shipment from the factory. Agilent Technologies further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology (formerly National Bureau of Standards), to the extent allowed by that organization's calibration facility, and to the calibration facilities of other International Standards Organization members.

Warranty

This Agilent Technologies product is warranted against defects in materials and workmanship for a period of one (1) year from date of shipment. Duration and conditions of warranty for this product may be superseded when the product is integrated into (becomes a part of) other Agilent products. During the warranty period, Agilent Technologies will, at its option, either repair or replace products which prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by Agilent Technologies. Buyer shall prepay shipping charges to Agilent and Agilent shall pay shipping charges to return the product to Buyer. However, Buyer shall pay all shipping charges, duties, and taxes for products returned to Agilent from another country.

Agilent warrants that its software and firmware designated by Agilent for use with a product will execute its programming instructions when properly installed on that product. Agilent does not warrant that the operation of the product, or software, or firmware will be uninterrupted or error free.

Limitation Of Warranty

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by Buyer, Buyer-supplied products or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

The design and implementation of any circuit on this product is the sole responsibility of the Buyer. Agilent does not warrant the Buyer's circuitry or malfunctions of Agilent products that result from the Buyer's circuitry. In addition, Agilent does not warrant any damage that occurs as a result of the Buyer's circuit or any defects that result from Buyer-supplied products.

NO OTHER WARRANTY IS EXPRESSED OR IMPLIED. Agilent SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

Exclusive Remedies

THE REMEDIES PROVIDED HEREIN ARE BUYER'S SOLE AND EXCLUSIVE REMEDIES. Agilent SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER BASED ON CONTRACT, TORT, OR ANY OTHER LEGAL THEORY.

Notice

The information contained in this document is subject to change without notice. Agilent Technologies MAKES NO WARRANTY OF ANY KIND WITH REGARD TO THIS MATERIAL, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. Agilent shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance or use of this material. This document contains proprietary information which is protected by copyright. All rights are reserved. No part of this document may be photocopied, reproduced, or translated to another language without the prior written consent of Agilent Technologies, Inc. Agilent assumes no responsibility for the use or reliability of its software on equipment that is not furnished by Agilent.

U.S. Government Restricted Rights

The Software and Documentation have been developed entirely at private expense. They are delivered and licensed as "commercial computer software" as defined in DFARS 252.227-7013 (Oct 1988), DFARS 252.211-7015 (May 1991) or DFARS 252.227-7014 (Jun 1995), as a "commercial item" as defined in FAR 2.101(a), or as "Restricted computer software" as defined in FAR 52.227-19 (Jun 1987)(or any equivalent agency regulation or contract clause), whichever is applicable. You have only those rights provided for such Software and Documentation by the applicable FAR or DFARS clause or the Agilent standard software agreement for the product involved.

Agilent E1351A/52A/53A/57A/58A FET Multiplexer Module Service Manual Edition 2 Rev 2


Copyright © 1996-2006 Agilent Technologies, Inc. All Rights Reserved.

Printing History

The Printing History shown below lists all Editions and Updates of this manual and the printing date(s). The first printing of the manual is Edition 1. The Edition number increments by 1 whenever the manual is revised. Updates, which are issued between Editions, contain replacement pages to correct the current Edition of the manual. Updates are numbered sequentially starting with Update 1. When a new Edition is created, it contains all the Update information for the previous Edition. Each new Edition or Update also includes a revised copy of this printing history page. Many product updates or revisions do not require manual changes and, conversely, manual corrections may be done without accompanying product changes. Therefore, do not expect a one-to-one correspondence between product updates and manual updates.

Edition 1	May 1993
Edition 2 (Part Number E1351-90011).	June 1996
Edition 2 Rev 2 (Part Number E1351-90011)	June 2006

Safety Symbols

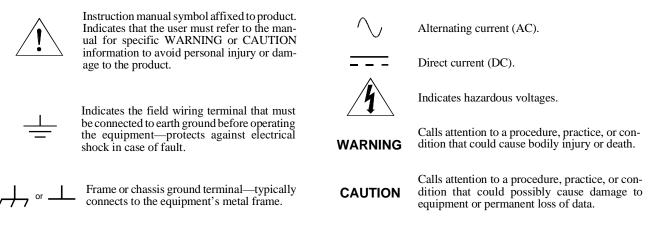

WARNINGS

The following general safety precautions must be observed during all phases of operation, service, and repair of this product. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the product. Agilent Technologies assumes no liability for the customer's failure to comply with these requirements.

Ground the equipment: For Safety Class 1 equipment (equipment having a protective earth terminal), an uninterruptible safety earth ground must be provided from the mains power source to the product input wiring terminals or supplied power cable.

DO NOT operate the product in an explosive atmosphere or in the presence of flammable gases or fumes.

For continued protection against fire, replace the line fuse(s) only with fuse(s) of the same voltage and current rating and type. DO NOT use repaired fuses or short-circuited fuse holders.

Keep away from live circuits: Operating personnel must not remove equipment covers or shields. Procedures involving the removal of covers or shields are for use by service-trained personnel only. Under certain conditions, dangerous voltages may exist even with the equipment switched off. To avoid dangerous electrical shock, DO NOT perform procedures involving cover or shield removal unless you are qualified to do so.

DO NOT operate damaged equipment: Whenever it is possible that the safety protection features built into this product have been impaired, either through physical damage, excessive moisture, or any other reason, REMOVE POWER and do not use the product until safe operation can be verified by service-trained personnel. If necessary, return the product to an Agilent Technologies Sales and Service Office for service and repair to ensure that safety features are maintained.

DO NOT service or adjust alone: Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

DO NOT substitute parts or modify equipment: Because of the danger of introducing additional hazards, do not install substitute parts or perform any unauthorized modification to the product. Return the product to an Agilent Technologies Sales and Service Office for service and repair to ensure that safety features are maintained.



Manufacturer's Name: Manufacturer's Address:

Agilent Technologies, Incorporated $815 - 14^{th}$ St. SW Loveland, Colorado 80537 USA

Declares, that the product

Agilent Technologies

Product Name:	16 Channel FET Multiplexer
Model Number:	E1351A
Product Options:	This declaration covers all options of the above product(s).

Conforms with the following European Directives:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC (including 93/68/EEC) and carries the CE Marking accordingly.

Conforms with the following product standards:

EMC	Standard	Limit
	CISPR 11:1990 / EN 55011:1991 EN50082-1 :1992	Group 1 Class A
	IEC 1000-4-2 :1995	4kV CD, 8kV AD
	IEC 1000-4-3 :1995	3 V/m
	IEC 1000-4-4 :1995	0.5kV signal lines, 1kV power lines
	The produt was tested in a typical configuration with Agilent Technol systems	logies or Hewlett-Packard Company test

Safety

IÉC 1010-1:1990+A2:1996 / EN 61010-1:1993 Canada: CSA C22.2 No. 1010.1:1992 UL 3111-1 : 1994

3 May 2001

Date

Ray Corson Product Regulations Program Manager



Manufacturer's Name:Agilent Technologies, IncorporatedManufacturer's Address:815 – 14th St. SWLoveland, Colorado 80537USA

Declares, that the product

Agilent Technologies

Product Name:	32 Channel Single Ended FET Multiplexer
Model Number:	E1352A
Product Options:	This declaration covers all options of the above product(s).

Conforms with the following European Directives:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC (including 93/68/EEC) and carries the CE Marking accordingly.

Conforms with the following product standards:

EMC	Standard	Limit
	CISPR 11:1990 / EN 55011:1991 EN50082-1 :1992	Group 1 Class A
	IEC 1000-4-2 :1995	4kV CD, 8kV AD
	IEC 1000-4-3 :1995	3 V/m
	IEC 1000-4-4 :1995	0.5kV signal lines, 1kV power lines
	The produt was tested in a typical configuration with systems	Agilent Technologies or Hewlett-Packard Company test
Catate	IEC 1010 1:1000 A2:1006 / EN 61010 1:1002	

Safety

systems IEC 1010-1:1990+A2:1996 / EN 61010-1:1993 Canada: CSA C22.2 No. 1010.1:1992 UL 3111-1 : 1994

3 May 2001

Date

Ray Corson Product Regulations Program Manager



Manufacturer's Name:	Agilent Technologies
Manufacturer's Address:	815 – 14 th St. SW
	Loveland, Colorado

Agilent Technologies

Agilent Technologies, Incorporated 815 – 14th St. SW Loveland, Colorado 80537 USA

Declares, that the product

Product Name:	16 Channel T/C FET Multiplexer
Model Number:	E1353A
Product Options:	This declaration covers all options of the above product(s).

Conforms with the following European Directives:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC (including 93/68/EEC) and carries the CE Marking accordingly.

Conforms with the following product standards:

EMC	Standard	Limit
	CISPR 11:1990 / EN 55011:1991 EN50082-1 :1992	Group 1 Class A
	IEC 1000-4-2 :1995	4kV CD, 8kV AD
	IEC 1000-4-3 :1995	3 V/m
	IEC 1000-4-4 :1995	0.5kV signal lines, 1kV power lines
	The produt was tested in a typical configuration with systems	Agilent Technologies or Hewlett-Packard Company test

Safety

systems IEC 1010-1:1990+A2:1996 / EN 61010-1:1993 Canada: CSA C22.2 No. 1010.1:1992 UL 3111-1 : 1994

3 May 2001

Date

Ray Corson Product Regulations Program Manager



Manufacturer's Name:Agilent Technologies, IncorporatedManufacturer's Address:815 – 14th St. SWLoveland, Colorado 80537USA

Agilent Technologies

Declares, that the product

Product Name:	8 Channel 120 Ohm Strain Relay FET
Model Number:	E1357A
Product Options:	This declaration covers all options of the above product(s).

Conforms with the following European Directives:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC (including 93/68/EEC) and carries the CE Marking accordingly.

Conforms with the following product standards:

EMC	Standard	Limit
	CISPR 11:1990 / EN 55011:1991 EN50082-1 :1992	Group 1 Class A
	IEC 1000-4-2 :1995	4kV CD. 8kV AD
	IEC 1000-4-3 :1995	3 V/m
	IEC 1000-4-4 :1995	0.5kV signal lines, 1kV power lines
	The produt was tested in a typical configuration with systems	Agilent Technologies or Hewlett-Packard Company test
0 - (- (IEC 1010 1:1000: A2:1006 / EN 61010 1:1002	

Safety

systems IEC 1010-1:1990+A2:1996 / EN 61010-1:1993 Canada: CSA C22.2 No. 1010.1:1992 UL 3111-1 : 1994

3 May 2001

Date

Ray Corson Product Regulations Program Manager



Manufacturer's Name:Agilent Technologies, IncorporatedManufacturer's Address:815 – 14th St. SWLoveland, Colorado 80537USA

Agilent Technologies

Declares, that the product

Product Name:	8 Channel 350 Ohm Strain Relay FET
Model Number:	E1358A
Product Options:	This declaration covers all options of the above product(s).

Conforms with the following European Directives:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC (including 93/68/EEC) and carries the CE Marking accordingly.

Conforms with the following product standards:

EMC	Standard	Limit
	CISPR 11:1990 / EN 55011:1991 EN50082-1 :1992	Group 1 Class A
	IEC 1000-4-2 :1995	4kV CD, 8kV AD
	IEC 1000-4-3 :1995	3 V/m
	IEC 1000-4-4 :1995	0.5kV signal lines, 1kV power lines
	systems	Agilent Technologies or Hewlett-Packard Company test
0 - (- 1	IEC 4040 4:4000; AD:4000 / EN 04040 4:4000	

Safety

systems IEC 1010-1:1990+A2:1996 / EN 61010-1:1993 Canada: CSA C22.2 No. 1010.1:1992 UL 3111-1 : 1994


3 May 2001

Date

Ray Corson Product Regulations Program Manager

Agilent 75000 Series B Service Documentation

Suggested Sequence to Use Manuals

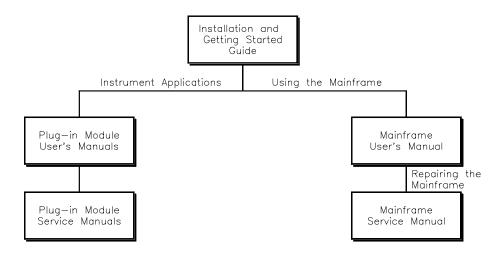

Manual Descriptions

Installation and Getting Started Guide. This manual contains step-by-step instructions for all aspects of plug-in module and mainframe installation. Introductory programming information and examples are also included.

Mainframe User's Manual. This manual contains programming information for the mainframe, front panel operation information (for the Agilent E1301B mainframe), and general programming information for instruments installed in the mainframe.

Plug-In Module User's Manuals. These manuals contain plug-in module programming and configuration information. Each manual contains examples for the most-used module functions, and a complete SCPI command reference for the plug-in module.

Mainframe Service Manual. This manual contains service information for the mainframe. It contains information for ordering replaceable parts and exchanging assemblies. Information and procedures for performance verification, adjustment, preventive maintenance, troubleshooting, and repair are also included.

Plug-In Module Service Manuals. These manuals contain plug-in module service information. Each manual contains information for exchanging the module and/or ordering replaceable parts. Depending on the module, information and procedures for functional verification, operation verification, performance verification, adjustment, preventive maintenance, troubleshooting, and repair are also provided.

Manual Overview

This manual shows how to service the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexers. Consult the appropriate *FET Multiplexer User's Manual* for additional information on installing, configuring, and operating each FET Multiplexer. Consult the appropriate mainframe user's manual for information on configuring and operating the mainframe.

Manual Content

Chapter	Title	Content
1	General Information	Provides a basic description and lists the test equipment required for service.
2	Verification Tests	Functional verification, operation verification, and performance verification tests.
3	Replaceable Parts	Lists replaceable parts for the module.
4	Service	Procedures to aid in fault isolation and repair of the module.

Table of Contents

Chapter 1 — General Information

Introduction
Safety Considerations
Warnings 1-2 Cautions 1-3
FET Multiplexer Description
Agilent E1351A Description
Agilent E1352A Description
Agilent E1353A Description
Agilent E1357ADescription
Agilent E1358A Description
FET Multiplexer Specifications
FET Multiplexer Environment 1-5 FET Multiplexer Social Number 1-5
FET Multiplexer Serial Numbers
FET Multiplexer Options
Recommended Test Equipment
Inspection/Shipping 1-6
Initial Inspection
Shipping Guidelines

Chapter 2 — Verification Tests

Introduction 2-1 Test Conditions/Procedures 2-1 Performance Test Record 2-1 Verification Test Examples 2-1
FunctionalVerification Test 2-2 Procedure 2-2 Example 2-2
Operation Verification Test
Performance Verification Tests 2-3 Test Fixture 2-3 Test 2-1: Closed Channel Resistance Test 2-4 Test 2-2: Leakage Test 2-12
Performance Test Record2-22Test Limits2-22Measurement Uncertainty2-22Test Accuracy Ratio (TAR)2-23

Chapter 3 — Replaceable parts

Introduction		•	•					•	•	•	•	 •	•	•	•	•	•	•	•	•	•	•		 3-1
Replaceable Parts Lists		•		•	•			•		•	•	 •	•	•	•				•	•	•	•	•	 3-1
Exchange Assembly		•		•				•		•	•	 •	•		•		•		•	•	•	•		 3-1
Mechanical Parts Locator	s.	•		•	•			•		•	•	 •	•			•	•	•	•	•	•	•		 3-5

Chapter 4 — Service

Introduction 4-1 Equipment Required 4-1 Service Aids 4-1 FET Multiplexer Description 4-1
Repair Strategy
Troubleshooting Techniques 4-6 Identifying the Problem 4-6 Making Visual Checks 4-7 Testing the Module 4-7
Repair and Maintenance Guidelines 4-8 ESD Precautions 4-8 Soldering Printed Circuit Boards 4-8 Post-Repair Safety Checks 4-8


Appendix A— Verification Tests - C Programs

Functional Verification Test	A-1
Example: Self Test	A-1
Performance Verification Tests	A-2
Example: Closed Channel Resistance Test	A-2
Example: Leakage Current Test	A-6

Chapter 1 General Information

Introduction

This manual contains information required to test, troubleshoot, and repair the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexers. See the appropriate *User's Manual* for additional information on the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A. Figure 1-1 shows the FET Multiplexers.

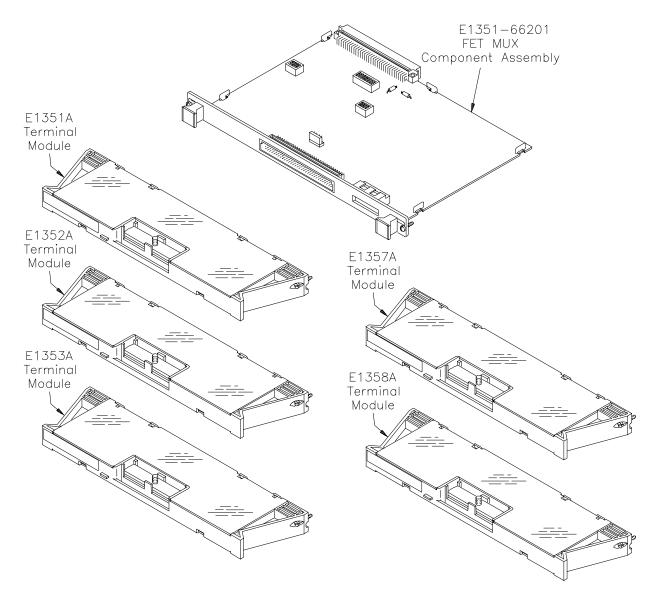



Safety Considerations	This product is a Safety Class I instrument that is provided with a protective earth terminal when installed in the mainframe. Check the mainframe, FET Multiplexer, Terminal Block, and all related documentation for safety markings and instructions before operation or service.
	Refer to the WARNINGS page (page ii) in this manual for a summary of safety information. Safety information for preventive maintenance, testing, and service follows and is also found throughout this manual.
Warnings	This section contains WARNINGS which must be followed for your protection when performing equipment maintenance or repair.
WARNING	SERVICE-TRAINED PERSONNEL ONLY. The information in this manual is for service-trained personnel who are familiar with electronic circuitry and are aware of the hazards involved. To avoid personal injury or damage to the instrument, do not perform procedures in this manual or do any servicing unless you are qualified to do so.
	CHECK MAINFRAME POWER SETTINGS. Before applying power, verify that the mainframe setting matches the line voltage and that the correct fuse is installed. An uninterruptible safety earth ground must be provided from the main power source to the supplied power cord set.
	GROUNDING REQUIREMENTS. Interruption of the protective (grounding) conductor (inside or outside the mainframe) or disconnecting the protective earth terminal will cause a potential shock hazard that could result in personal injury. (Grounding one conductor of a two-conductor outlet is not sufficient protection.)
	IMPAIRED PROTECTION. Whenever it is likely that instrument protection has been impaired, the mainframe must be made inoperative and be secured against any unintended operation.
	REMOVE POWER IF POSSIBLE. Some procedures in this manual may be performed with power supplied to the mainframe while protective covers are removed. Energy available at many points may, if contacted, result in personal injury. (If maintenance can be performed without power applied, the power should be removed.)

WARNING	USING AUTOTRANSFORMERS. If the mainframe is to be energized via an autotransformer (for voltage reduction) make sure the common terminal is connected to neutral (that is, the grounded side of the main's supply).
	CAPACITOR VOLTAGES. Capacitors inside the mainframe may remain charged even when the mainframe has been disconnected from its source of supply.
	USE PROPER FUSES. For continued protection against fire hazard, replace the line fuses only with fuses of the same current rating and type (such as normal blow, time delay, etc.). Do not use repaired fuses or short-circuited fuseholders.
Cautions	This section contains CAUTIONS which must be followed to avoid damage to the equipment when performing instrument maintenance or repair.
CAUTION	MAXIMUM VOLTAGE/CURRENT. The maximum voltage that may be applied between any connector pin and any other point, shield, or chassis is 15 VPeak.
	STATIC ELECTRICITY. Static electricity is a major cause of component failure. To prevent damage to the electrical components in the FET Multiplexer, observe anti-static techniques whenever working on a FET Multiplexer.

FET Multiplexer Description	The Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexer is an "instrument" in a VXIbus mainframe. As such, each FET Multiplexer is assigned an error queue, input and output buffers, and a status register.
NOTE	Instruments are based on the logical addresses of the plug-in modules. See the Agilent 75000 Series B Installation and Getting Started Guide to set the addresses to create an instrument.
	The FET Multiplexer Module consists of a component assembly and a terminal block. There are five different terminal blocks, one for each application. The component assembly is the same for all applications. The applications supported by the component assembly are:
	 Agilent E1351A 16-Channel FET Multiplexer Agilent E1352A 32-Channel Single Ended FET Multiplexer Agilent E1353A 16-Channel Thermocouple FET Multiplexer Agilent E1357A 8-Channel 120 Ω Strain Gage FET Multiplexer Agilent E1358A 8-Channel 350 Ω Strain Gage FET Multiplexer
	Each terminal block configures the component assembly to the appropriate type of switch. The terminal card also contains the model identification code and installation of the terminal card before applying mainframe power ensures that the type of switch is properly identified. Optionally, the model identification can be set on the component assembly to allow it to be correctly identified without a terminal card installed.
Agilent E1351A Description	The Agilent E1351A provides high speed switching for up to 16 channels. The channels are numbered 00 to 15. Each channel provides connections for High (HI), Low (LO), and Guard (G), although only High and Low are switched. Guard for each channel is connected to chassis ground through a $10 \text{ k} \Omega$ resistor.
Agilent E1352A Description	The Agilent E1352A provides high-speed switching for up to 32 channels. The channels are numbered 00 to 31. A High (HI) connection is provided for each channel. Low (LO) and Guard (G) are common for all channels.
Agilent E1353A Description	The Agilent E1353A is identical to the Agilent E1351A, but contains a temperature reference thermistor on the terminal block to allow thermocouple temperature measurements when combined with either the Agilent E1326A or E1411B Multimeters.

Agilent E1357A Description	The Agilent E1357A provides up to eight channels of strain gage switching. Strain gage measurements are supported in 1/4 bridge, 1/2 bridge, and full bridge measurements with 120 Ω completion resistors. A strain gage excitation power supply is also provided.
Agilent E1358A Description	The Agilent E1358A is identical to the Agilent E1357A except the strain gage completion resistors are 350 Ω
FET Multiplexer Specifications	See <i>Appendix A</i> of the appropriate <i>User's Manual</i> for Agilent E1351A, E1352A, E1353A, E1357A, and E1358A specifications. These specifications are the performance standards or limits against which the instrument may be tested.
FET Multiplexer Environment	The recommended operating environment for the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexer is:

Environment	Temperature	Humidity
Operating	0°C to +55°C	<65% relative (0°C to +40°C)
Storage and Shipment	-40°C to +75°C	<65% relative (0°C to +40°C)

FET Multiplexer Serial Numbers

FET Multiplexers covered by this manual are identified by a serial number prefix listed on the title page. Agilent Technologies uses a two-part serial number in the form XXXXAYYYYY, where XXXX is the serial prefix, A is the country of origin (A=USA), and YYYYY is the serial suffix. The serial number prefix identifies a series of identical instruments. The serial number suffix is assigned sequentially to each instrument.

The serial number plate is located on the backplane connector. If the serial number prefix of your instrument is greater than the one listed on the title page, a Manual Update (as required) will explain how to adapt this manual to your instrument.

FET Multiplexer
OptionsThere are no electrical or mechanical options available for the Agilent
E1351A, E1352A, E1353A, E1357A, or E1358A FET Multiplexers.

Recommended Test Equipment

Table 1-1 lists the test equipment recommended for testing, adjusting, and servicing the FET Multiplexers. Essential requirements for each piece of test equipment are described in the Requirements column.

Instrument	Requirements	Recommended Model	Use*
Controller, GPIB	GPIB compatibility as defined by IEEE Standard 488-1987 and the identical ANSI Standard MC1.1: SH1, AH1, T2, TE0, L2, LE0, SR0, RL0, PP0, DC0, DT0, and C1, 2, 3, 4, 5.	HP 9000 Series 300 or IBM Compatible PC with BASIC	F,O, P,T
Mainframe	Compatible with FET Multiplexer	Agilent E1300B, E1301B, E1302A or E1401B, E1421A (requires E1405A/B)	F,O, P,T
Digital Multimeter	2-Wire Ohms (up to 10 k Ω) DC Volts (to 0.01 mV)	Agilent 3458A or Agilent 34401A	O,P,T
Power Supply	+10 Vdc ± 0.1 V	Agilent 6214C	Ρ, Τ
Resistor	100 k $\Omega \pm$ 1%	Agilent PN 0757-0465	Ρ, Τ

Table 1-1. Recommended Test Equipment

* F = Functional Verification Tests, O = Operation Verification Tests, P = Performance Verification Tests, T = Troubleshooting

Inspection/ Shipping

This section contains initial (incoming) inspection and shipping guidelines for the FET Multiplexer.

InitialUse the steps in Figure 1-2 as guidelines to perform initial inspection of aInspectionFET Multiplexer. Performance Verification tests are optional.

WARNING

To avoid possible hazardous electrical shock, do not perform electrical tests if there are signs of shipping damage to the shipping container or to the instrument.

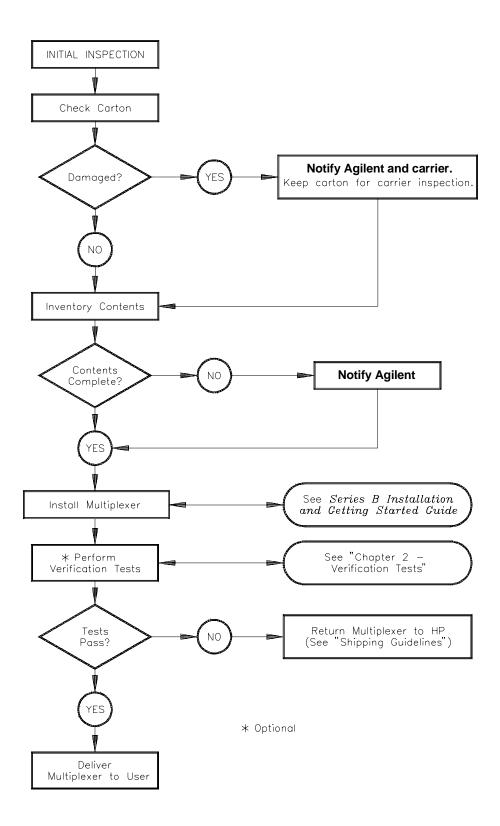


Figure 1-2. Initial (Incoming) Inspection Guidelines

Shipping Guidelines

Follow the steps in Figure 1-3 to return a FET Multiplexer to an Agilent Technologies Sales and Support Office or Service Center.

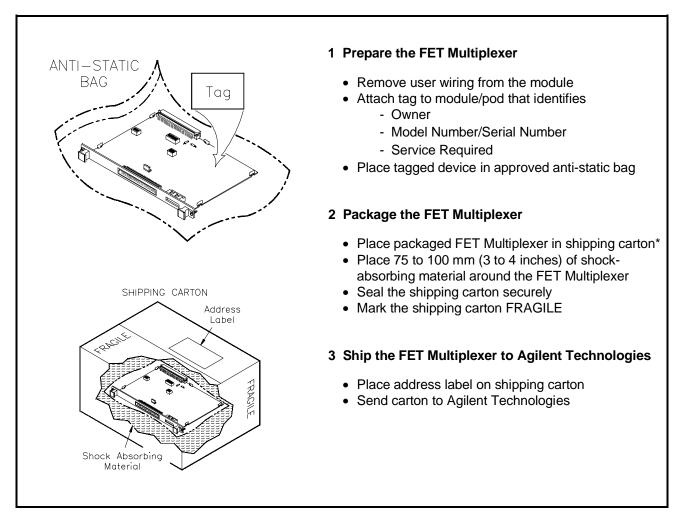


Figure 1-3. Packaging/Shipping Guidelines

* We recommend that you use the same shipping materials as those used in factory packaging (available from Agilent Technologies). For other (commercially-available) shipping materials, use a double wall-carton with minimum 2.4 MPa (350 psi) test.

Chapter 2 Verification Tests

Introduction	This chapter describes the verification tests for the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A. The three levels of test procedures described in this chapter are used to verify that the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A:
	 is functional (Functional Verification Test) meets selected testable specifications (Operation Verification) meets all testable specifications (Performance Verification)
Test Conditions/ Procedures	See Table 1-1 for test equipment requirements. You should complete the Performance Verification tests at least once a year. For heavy use or severe operating environments, perform the tests more often. The verification tests assume that the person performing the tests understands how to operate the mainframe, the FET Multiplexer, and the specified test equipment. The test procedures do not specify equipment settings for test equipment except in general terms. It is assumed that a qualified, service-trained technician will select and connect the fixtures, adapters, and probes required for the test.
Performance Test Record	The results of each Performance Verification test may be recorded in Table 2-1, <i>Performance Test Record</i> , at the end of this chapter. You can make a copy of this form, if desired.
Verification Test Examples	Each verification test procedure includes an example program that performs the test. All example programs assume the following configuration:
	 HP 9000 Series 200/300 computer BASIC programming language FET Multiplexer address 70914 FET Multiplexer card number 1

• Agilent 3458A Digital Multimeter (DMM)

The Functional Verification Test for the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexers consists of sending the *IDN? command and checking the response. This test can be used to verify that the FET Multiplexer is connected properly and is responding to a basic command.			
1. Verify that the FET Multiplexer is properly installed in the mainframe			
2. Verify that the terminal block or test fixture is properly connected to the Multiplexer			
3. Verify that the mainframe has passed its power-on test			
4. Send *IDN? to the FET Multiplexer (see example following)			
5. The return should be as follows (revision number may vary):			
HEWLETT-PACKARD,SWITCHBOX,0,A.07.00			
If the primary address setting, secondary address setting, or the interface select code is set incorrectly, the FET Multiplexer will not respond. Verify proper address selection before troubleshooting.			
ExampleAn example follows which uses an HP 9000 Series 300 computer with BASIC and a FET Multiplexer address of 70914.10DIM A\$[100]20OUTPUT 70914;"*IDN?"20OUTPUT 70914;A\$30ENTER 70914;A\$40PRINT A\$50END			

Operation Verification Test	The procedures in this section are used to provide a high level of confidence that the FET Multiplexer is meeting published specifications. The Operation Verification Test is a subset of the Performance Verification Tests and is suitable for checkout after performing repairs. The Operation Verification Test is performed by completing the Closed Channel Resistance Test (Test 2-1) as described in the Performance Verification Test procedures. This test is usually sufficient to verify that the FET Multiplexer is meeting its specifications.
Performance Verification Tests	The procedure in this section is used to test the FET Multiplexer's electrical performance using the specifications in <i>Appendix A</i> — <i>Specifications</i> of the appropriate <i>FET Multiplexer User's Manual</i> as the performance standard. There are two performance verification tests; <i>Test 2-1: Closed channel Resistance Test</i> , and <i>Test 2-2: Leakage Test</i> . These tests are suitable for incoming inspection, troubleshooting, and preventive maintenance.
Test Fixture	A Test Fixture is required to run the Performance Verification tests. Figure 2-1 shows the connections using an Agilent E1351A Terminal Block for the test fixture. The Agilent E1352A, E11353A, E1357A and E1358A Terminal Blocks are not recommended as test fixtures. You may want to order an extra terminal block to use as a test fixture, so you don't have to

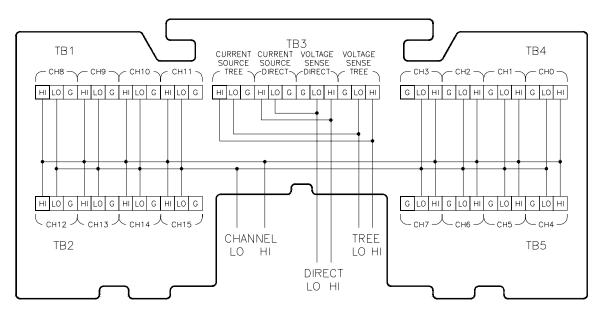


Figure 2-1. FET Multiplexer Test Fixture

re-wire each time the tests are performed. The Agilent E1351A terminal block and case assembly part number is E1351-80001.

This test first verifies that no FET switches are stuck in the on condition and

specification for the FET Multiplexer. The channel HI, channel LO, A Tree,

then verifies that all channels meet the closed channel resistance

Test 2-1: Closed Channel Resistance Test

HI Channel Measurements

1. Make Hardware Connections

• Turn mainframe power OFF

and B Tree switches are all independently tested.

- Connect DMM as shown in Figure 2-2
- Turn mainframe power ON

Agilent E1300B/E1301B

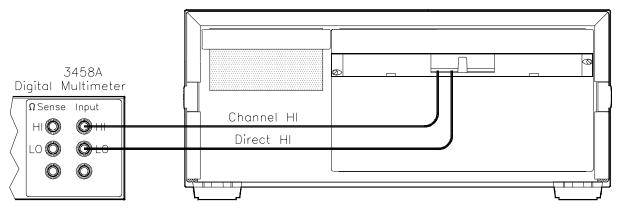


Figure 2-2. HI Channel Resistance Test Connections

- 2. Check for Stuck Channels
 - Send *RST to the FET Multiplexer to open all channels
 - Trigger the DMM with TRIG SGL and note reading
 - Verify the reading is greater than $10 \text{ k}\Omega$

3. Check HI Closed Channel Resistance


- Send CLOS (@*nn*00) to close channel 00, where *nn* is the card number (typically 01)
- Trigger the DMM with TRIG SGL and note the reading
- Enter the result in Table 2-1 for channel 00 HI
- Send OPEN (@nn00) to open channel 00, where nn is the card number
- 4. Repeat for Channels 01 through 15

- Repeat step 3 for channels 01 through 15
- Use CLOS (@*nncc*), where *nn* is the card number and *cc* is the channel number

LO Channel Measurements

1. Make Hardware Connections

- Turn mainframe power OFF
- Connect DMM as shown in Figure 2-3
- Turn mainframe power ON

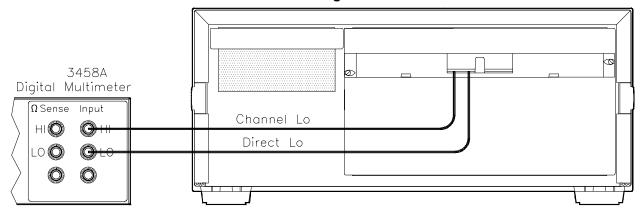

Agilent E1300B/E1301B

Figure 2-3. LO Channel Resistance Test Connections

2. Check for Stuck Channels

- Send *RST to the FET Multiplexer to open all channels
- Trigger the DMM with TRIG SGL and note reading
- Verify the reading is greater than $10 \text{ k}\Omega$

3. Check LO Closed Channel Resistance

- Send CLOS (@*nn*00) to close channel 00, where *nn* is the card number (typically 01)
- Trigger the DMM with TRIG SGL and note the reading
- Enter the result in Table 2-1 for channel 00 LO
- Send OPEN (@nn00) to open channel 00, where nn is the card number

4. Repeat for Channels 01 through 15

- Repeat step 3 for channels 01 through 15
- Use CLOS (@nncc) and OPEN (@nncc), where nn is the card number and cc is the channel number

Tree Switch HI Channel Measurements

1. Make Hardware Connections

- Turn mainframe power OFF
- Connect DMM as shown in Figure 2-4
- Turn mainframe power ON

Agilent E1300B/E1301B

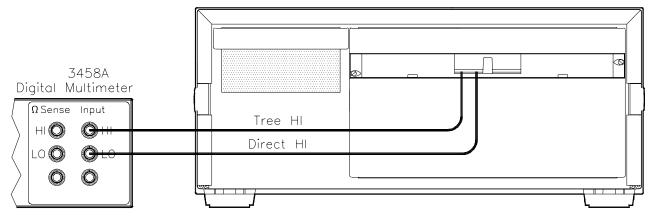


Figure 2-4. Tree HI Resistance Test Connections

- 2. Check for Stuck Channels
 - Send *RST to the FET Multiplexer to open all channels
 - Trigger the DMM with TRIG SGL and note reading
 - Verify the reading is greater than $10 \text{ k}\Omega$
- 3. Check Tree Switch HI Closed Channel Resistance
 - Send SCAN:PORT ABUS to enable the tree switches
 - Send CLOS (@*nn*00) to close channel 00 and the A tree switch, where *nn* is the card number (typically 01)
 - Trigger the DMM with TRIG SGL and note the reading
 - Enter the result in Table 2-1 for Tree A HI
 - Send OPEN (@nn00) to open channel 00, where nn is the card number
 - Send CLOS (@*nn*15) to close channel 15 and the B tree switch, where *nn* is the card number
 - Trigger the DMM with TRIG SGL and note the reading
 - Enter the result in Table 2-1 for Tree B HI
 - Send *RST to the FET Multiplexer

Tree Switch LO Channel Measurements

1. Make Hardware Connections

- Turn mainframe power OFF
- Connect DMM as shown in Figure 2-5
- Turn mainframe power ON

Agilent E1300B/E1301B

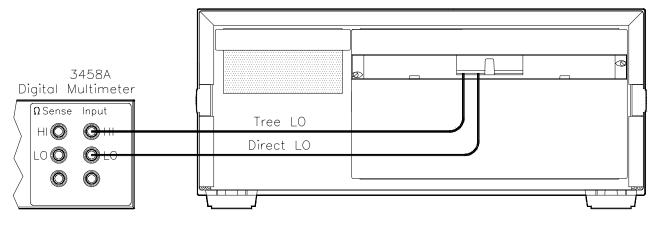


Figure 2-5. Tree LO Resistance Test Connections

2. Check for Stuck Channels

- Send *RST to the FET Multiplexer to open all channels
- Trigger the DMM with TRIG SGL and note reading
- Verify the reading is greater than $10 \text{ k}\Omega$

3. Check Tree Switch LO Closed Channel Resistance

- Send SCAN:PORT ABUS to enable the tree switches
- Send CLOS (@*nn*00) to close channel 00 and the A tree switch, where *nn* is the card number (typically 01)
- Trigger the DMM with TRIG SGL and note the reading
- Enter the result in Table 2-1 for Tree A LO
- Send OPEN (@nn00) to open channel 00, where nn is the card number
- Send CLOS (@*nn*15) to close channel 15 and the B tree switch, where *nn* is the card number
- Trigger the DMM with TRIG SGL and note the reading
- Enter the result in Table 2-1 for Tree B LO
- Send *RST to the FET Multiplexer

Example: Closed Channel Resistance Test

This example performs a closed channel resistance test of all measurement paths. If a FET on resistance is >3.1 k Ω , the program prints a message indicating which channel has failed. Before the closed channel measurement, the program checks for stuck channels. If a stuck channel is found, the program prints a message and halts.

- 10! RE-SAVE "CLOS_TEST"
- 20 ASSIGN @Dmm TO 722
- 30 ASSIGN @Mux TO 70914
- 40 DISP CHR\$(129)
- 50 DIM Result(1,15), Tree(1,1), Path\$(1)[4], Cc\$[2], Ch\$[2]
- 60 DATA HI,LO
- 70 READ Path\$(*)
- 80 Cc\$ = "01" ! Card number
- 90 !
- 100 ! Start test
- 110 !
- 120 CLEAR SCREEN
- 130 PRINT "Install Component Assembly and Test Fixture"
- 140 PRINT
- 150 PRINT " 1. Turn mainframe and Agilent 3458A DMM power OFF"
- 160 PRINT " 2. Connect GPIB cable between mainframe and DMM"
- 170 PRINT " 3. Install component assembly into mainframe"
- 180 PRINT " 4. Attach test fixture to component assembly"
- 190 PRINT " 5. Turn mainframe and DMM power ON"
- 200 PRINT " 6. Press Continue when ready to begin testing"
- 210 PAUSE
- 220 !
- 230 ! Measure closed channel resistance
- 240 !
- 250 FOR I = 0 TO 1
- 260 CLEAR SCREEN

270 PRINT TABXY(1,1), "Channel ";Path\$(I);" to Direct ";Path\$(I);" Measurements"

280 PRINT TABXY(1,3),"Connect DMM Input HI lead to Channel ";Path\$(I)

- 290 PRINT TABXY(1,4),"Connect DMM Input LO lead to Direct ";Path\$(I)
- 300 DISP "Press Continue when connections are complete"
- 310 PAUSE

!

- 320 OUTPUT @Dmm;"PRESET NORM;FUNC OHM"
- 330 OUTPUT @Mux;"*RST"
- 340
- 350 ! Check for stuck channels
- 360 !

370	OUTPUT @Dmm;"TRIG SGL"
380	ENTER @Dmm;Value
390	IF Value<10000 THEN
400	CLEAR SCREEN
410	PRINT "Measurement indicates a stuck channel"
420	PRINT "Correct the problem before proceeding"
430	STOP
440	END IF
450	CLEAR SCREEN
460	FOR J = 0 TO 15
470	IF J<10 THEN
480	Ch\$="0"&VAL\$(J)
490	ELSE
500	Ch\$=VAL\$(J)
510	END IF
520	OUTPUT @Mux;"CLOS (@"&Cc\$&Ch\$&")"
530	OUTPUT @Dmm;"TRIG SGL"
540	ENTER @Dmm;Result(I,J)
550	OUTPUT @Mux;"OPEN (@"&Cc\$&Ch\$&")"
560	IF Result(I,J)>3100 THEN
570 Paths	PRINT "Resistance for channel ";J;" "; \$(I);" is > 3.1 kOhms"
580	END IF
590	NEXT J
600	PRINT "Measurements complete for channel ";Path\$(I)
610	IF I=0 THEN
620	DISP "Press Continue for channel ";Path\$(I+1);" measurements"
630	PAUSE
640	END IF
650	NEXTI
660	PRINT "Measurements complete for channel HI and LO"
670	DISP "Press Continue for Tree Switch measurements"
680	PAUSE
690	!
700	! Tree Switch measurements
710	!
720	FOR I = 0 TO 1
730	CLEAR SCREEN
740 " me	PRINT TABXY(1,1), "Tree ";Path\$(I);" to Direct ";Path\$(I); asurements"
750	PRINT TABXY(1,3),"Connect DMM Input HI lead to Tree ";Path\$(I)
760	PRINT TABXY(1,4),"Connect DMM Input LO lead to Direct ";Path\$(I)
770	DISP "Press Continue when connections are complete"

780	PAUSE			
790	OUTPUT @Dmm;"PRESET NORM;FUNC OHM"			
800	OUTPUT @Mux;"*RST"			
810	!			
820	! Check for stuck tree switches			
830	!			
840	OUTPUT @Dmm;"TRIG SGL"			
850	ENTER @Dmm;Value			
860	IF Value<10000 THEN			
870	CLEAR SCREEN			
880	PRINT "Measurement indicates a stuck tree switch"			
890	PRINT "Correct the problem before proceeding"			
900	STOP			
910	END IF			
920	CLEAR SCREEN			
930	FOR J = 0 TO 1			
940	IF J=0 THEN			
950	Ch\$="00"			
960	ELSE			
970	Ch\$="15"			
980	END IF			
990	OUTPUT @Mux;"SCAN:PORT ABUS"			
1000	OUTPUT @Mux;"CLOS (@"&Cc\$&Ch\$&")"			
1010	OUTPUT @Dmm;"TRIG SGL"			
1020	ENTER @Dmm;Tree(I,J)			
1030	1030 OUTPUT @Mux;"OPEN (@"&Cc\$&Ch\$&")"			
1040	IF Tree(I,J)>3100 THEN			
1050	IF Ch\$="00" THEN			
1060 " is > 3	1060 PRINT "Resistance for A Tree Switch ";Path\$(I); " is > 3.1 kOhms"			
1070	ELSE			
1080 " is > 3				
1090	END IF			
1100	END IF			
1110	NEXT J			
1120	PRINT "Measurements complete for tree switch ";Path\$(I)			
1130	IF I=0 THEN			
1140 DISP "Press Continue for Tree Switch ";Path\$(I+1); " measurements"				
1150	PAUSE			
1160	END IF			
1170 I	NEXTI			

1180 PRINT "Closed channel resistance measurements complete"				
1190				
	PAUSE			
1210	CLEAR SCREEN			
1220	!			
1230	! Print results			
1240	!			
	Format1:IMAGE "Channel DD," Ohms"	",DD,"	HI ",DDDDD," Ohms	LO
	Format2:IMAGE "Tree DD," Ohms"	",K,"	HI ",DDDDD," Ohms	LO
1270	PRINT "Closed channel re	esistance m	neasurement results"	
1280	FOR J=0 TO 15			
1290	PRINT USING Format1;	J,Result(0,	J),Result(1,J)	
1300	NEXT J			
1310	PRINT			
1320	PRINT USING Format2;"/	A",Tree(0,0),Tree(0,1)	
1330	PRINT USING Format2;"E	3",Tree(1,0),Tree(1,1)	
1340	END			

Typical Result

Closed chan	nel resistar	nce measurement res	sults		
Channel	0	HI	989 Ohms	LO	1004 Ohms
Channel	1	HI	991 Ohms	LO	979 Ohms
Channel	2	HI	1001 Ohms	LO	989 Ohms
Channel	3	HI	990 Ohms	LO	1000 Ohms
Channel	4	HI	988 Ohms	LO	999 Ohms
Channel	5	HI	1002 Ohms	LO	995 Ohms
Channel	6	HI	1010 Ohms	LO	1000 Ohms
Channel	7	HI	998 Ohms	LO	998 Ohms
Channel	8	HI	1006 Ohms	LO	1008 Ohms
Channel	9	HI	1000 Ohms	LO	1002 Ohms
Channel	10	HI	995 Ohms	LO	988 Ohms
Channel	11	HI	999 Ohms	LO	990 Ohms
Channel	12	HI	1000 Ohms	LO	1000 Ohms
Channel	13	HI	989 Ohms	LO	991 Ohms
Channel	14	HI	979 Ohms	LO	989 Ohms
Channel	15	HI	1004 Ohms	LO	995 Ohms
Tree	А	Н	988 Ohms	LO	991 Ohms
Tree	В	HI	992 Ohms	LO	998 Ohms


Test 2-2: Leakage Test

The test verifies the input impedance by measuring the voltage drop across a known resistor in series with the input impedance. Leakage is measured from HI to LO, HI to Chassis, and LO to Chassis. Because of the solid state nature of the switches and input protection, the leakage is measured at both +10 Vdc and -10 Vdc.

HI to LO Leakage

1. Make Hardware Connections

- Turn power supply, DMM, and mainframe power OFF
- Connect DMM, power supply, and resistor as shown in Figure 2-6
- Turn power supply, DMM, and mainframe power ON
- Set power supply output to $+10 \text{ Vdc} \pm 0.1 \text{ Vdc}$

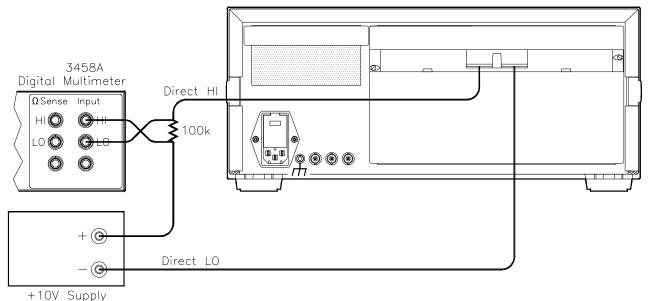

Agilent E1300B/E1301B

Tov Supply

Figure 2-6. Positive HI to LO Leakage Connections

2. Check Direct Terminals Leakage

- Send *RST to FET Multiplexer
- Send TRIG SGL to DMM
- Record the DMM reading in Table 2-1 Positive Polarity, HI to LO, Direct
- The DMM measurement should be less than 0.010 Vdc. A measurement out of this range indicates a failure of the FET Multiplexer and troubleshooting/repair/replacement procedures, described in Chapter 4, should be performed before proceeding with Test 2-2

- 3. Check Channels Leakage
 - Send CLOS(@*nn*00) to the FET Multiplexer to close channel 00, where *nn* is card number (typically 01)
 - Send TRIG SGL to DMM
 - Record the DMM reading in Table 2-1 Positive Polarity, HI to LO, Channels
 - Send OPEN (@nn00) to the FET Multiplexer
- 4. Check Tree Leakage
 - Send SCAN:PORT ABUS to the FET Multiplexer to enable the Tree Switches
 - Send CLOS(@nn00) to the FET Multiplexer to close channel 00 and Tree Switch A, where nn is the card number (typically 01)
 - Send TRIG SGL to DMM
 - Record the DMM reading in Table 2-1 Positive Polarity, HI to LO, Tree A
 - Send OPEN (@nn00) to the FET Multiplexer
 - Send CLOS(@*nn*15) to the FET Multiplexer to close channel 15 and Tree Switch B
 - Send TRIG SGL to DMM
 - Record the DMM reading in Table 2-1 Positive Polarity, HI to LO, Tree B
 - Send *RST to the FET Multiplexer

5. Change Polarity

- Turn power supply and mainframe power OFF
- Connect DMM, power supply, and resistor as shown in Figure 2-7
- Turn power supply and mainframe power ON
- Set power supply output to ± 10 Vdc ± 0.1 Vdc

6. Repeat Steps 2 through 4

• Record all results in Table 2-1 as Negative Polarity, HI to LO

Agilent E1300B/E1301B

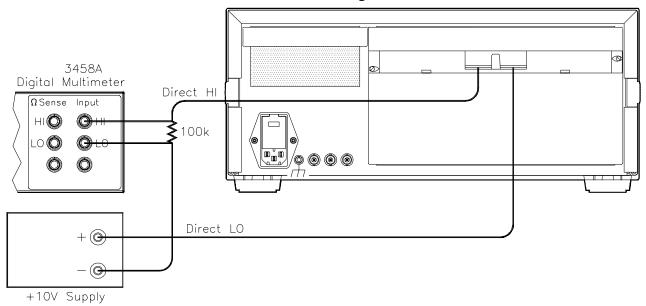


Figure 2-7. Negative HI to LO Leakage Connections

HI to Chassis Leakage

1. Make Hardware Connections

- Turn power supply and mainframe power OFF
- Connect DMM, power supply, and resistor as shown in Figure 2-8
- Turn power supply and mainframe power ON

2. Check Direct Terminals Leakage

- Send *RST to FET Multiplexer
- Send TRIG SGL to DMM
- Record the DMM reading in Table 2-1 Positive Polarity, HI to Chassis, Direct
- The DMM measurement should be less than 0.010 Vdc. A measurement out of this range indicates a failure of the FET Multiplexer

Agilent E1300B/E1301B

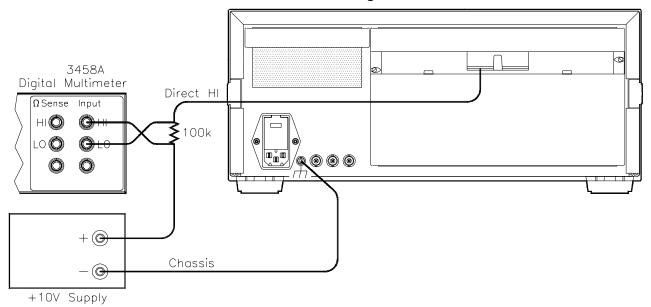


Figure 2-8. Positive HI to Chassis Leakage Connections

3. Check Channels Leakage

- Send CLOS(@*nn*00) to the FET Multiplexer, where *nn* is the channel number (typically 01)
- Send TRIG SGL to DMM
- Record the DMM reading in Table 2-1 Positive Polarity, HI to Chassis, Channels
- Send OPEN (@nn00) to the FET Multiplexer

4. Check Tree Leakage Current

- Send SCAN:PORT ABUS to the FET Multiplexer
- Send CLOS(@*nn*00) to the FET Multiplexer to close channel 00 and Tree A, where *nn* is the card number (typically 01)
- Send TRIG SGL to DMM
- Record the DMM reading in Table 2-1 Positive Polarity, HI to Chassis, Tree A
- Send OPEN (@nn00) to the FET Multiplexer


- Send CLOS(@*nn*15) to the FET Multiplexer to close channel 15 and tree B
- Send TRIG SGL to DMM
- Record the DMM reading in Table 2-1 Positive Polarity, HI to Chassis, Tree B
- Send *RST to the FET Multiplexer

5. Change Polarity

- Turn power supply and mainframe power OFF
- Connect DMM, power supply, and resistor as shown in Figure 2-9
- Turn power supply and mainframe power ON
- Set power supply output to $+10 \text{ Vdc} \pm 0.1 \text{ Vdc}$

6. Repeat Steps 2 through 4

• Record all results in Table 2-1 as Negative Polarity, HI to Chassis

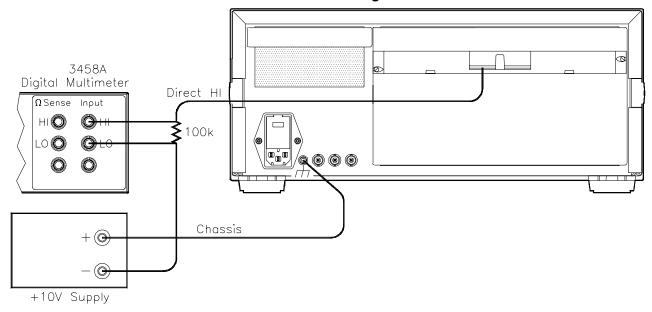


Agilent E1300B/E1301B

Figure 2-9. Negative HI to Chassis Leakage Connections

LO to Chassis Leakage

1. Make Hardware Connections

- Turn power supply and mainframe power OFF
- Connect DMM, power supply, and resistor as shown in Figure 2-10
- Turn power supply and mainframe power ON

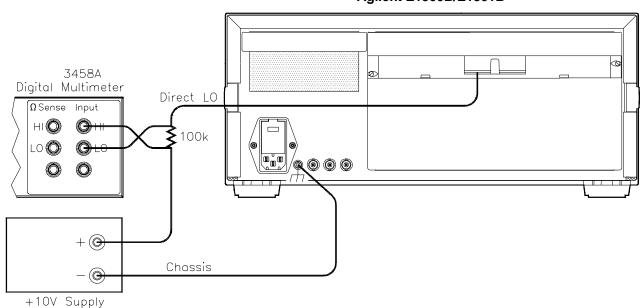

Agilent E1300B/E1301B

Figure 2-10. Positive LO to Chassis Leakage Connections

- 2. Check Direct Terminals Leakage Current
 - Send *RST to FET Multiplexer
 - Send TRIG SGL to DMM
 - Record the DMM reading in Table 2-1 Positive Polarity, LO to Chassis, Direct
 - The DMM measurement should be less than 0.010 Vdc. A measurement out of this range indicates a failure of the FET Multiplexer.
- 3. Check Channels Leakage
 - Send CLOS(@*nn*00) to the FET Multiplexer, where *nn* is the card number (typically 01)
 - Send TRIG SGL to DMM

- Record the DMM reading in Table 2-1 Positive Polarity, LO to Chassis, Channels
- Send OPEN (@nn00) to the FET Multiplexer

4. Check Tree Leakage Current


- Send SCAN:PORT ABUS to the FET Multiplexer
- Send CLOS(@nn00) to the FET Multiplexer to close channel 00 and Tree A, where nn is the card number (typically 01)
- Send TRIG SGL to DMM
- Record the DMM reading in Table 2-1 Positive Polarity, LO to Chassis, Tree A
- Send OPEN (@*nn*00) to the FET Multiplexer
- Send CLOS(@*nn*15) to the FET Multiplexer to close channel 15 and Tree B
- Send TRIG SGL to DMM
- Record the DMM reading in Table 2-1 Positive Polarity, LO to Chassis, Tree B
- Send *RST to the FET Multiplexer

5. Change Polarity

- Turn power supply and mainframe power OFF
- Connect DMM, power supply, and resistor as shown in Figure 2-11
- Turn power supply and mainframe power ON

6. Repeat Steps 2 through 4

• Record all results in Table 2-1 as Negative Polarity, LO to Chassis

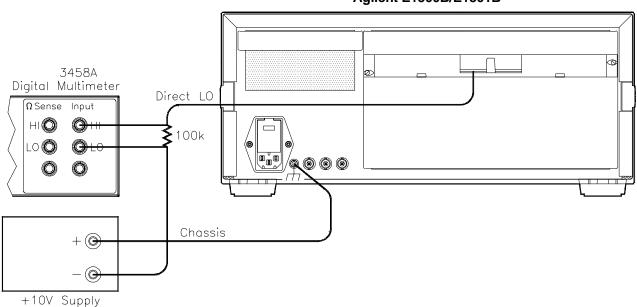

Agilent E1300B/E1301B

Figure 2-11. Negative LO to Chassis Leakage Connections

Example: Leakage
Current TestThis example performs a leakage test from HI to LO, HI to Chassis, and LO
to Chassis. If the leakage is too high (caused by a failure of the input
impedance), the test prints a message indicating which leakage path has
failed and halts.

- 10! RE-SAVE "LEAK_TEST"
- 20 ASSIGN @Dmm TO 722
- 30 ASSIGN @Mux TO 70914
- 40 DISP CHR\$(129)
- 50 DIM Result(5,3), Path\$(5,3)[16],Cc\$[2]
- 60 DATA Power Supply HI, Direct HI, LO, Direct LO
- 70 DATA Direct HI, Power Supply LO, HI, Direct LO
- 80 DATA Power Supply HI, Direct LO, LO, Chassis
- 90 DATA Direct HI, Power Supply LO, HI, Chassis
- 100 DATA Power Supply HI, Direct LO, LO, Chassis
- 110 DATA Direct LO, Power Supply LO, HI, Chassis
- 120 READ Path\$(*)
- 130 Cc\$="01" ! Card Number
- 140 CLEAR SCREEN
- 150 PRINT "Install component assembly and test fixture"
- 160 PRINT

180 190 200 210 220 230	PAUSE	Turn mainframe, power supply, and DMM power OFF" Connect GPIB cable between mainframe and DMM" Install component assembly into mainframe" Attach test fixture to component assembly" Turn mainframe and DMM power ON" Press Continue when ready to begin testing"
240	!	
	! Start Test	
		A
	OUTPUT @N	-
280		Dmm;"PRESET NORM;FUNC DCV"
290		
300	CLEAR S	
310 Input		I. Connect 100 kOhm resistor from DMM Input HI to DMM
320	PRINT "2	Connect DMM Input HI lead to ";Path\$(I,0)
330	PRINT "3	Connect DMM Input LO lead to ";Path\$(I,1)
340	PRINT "4	 Connect Power Supply ";Path\$(I,2);" to ";Path\$(I,3)
350	PRINT "5	5. Turn ON power supply and set output for +10 Vdc"
360	DISP "Pre	ss Continue when connections are complete"
370	PAUSE	
380	OUTPUT	@Dmm;"TRIG SGL"
390	ENTER @	2Dmm;Result (I,0)
400	IF Result ((I,0) > .01 THEN
410	PRINT	Γ "Direct path leakage out of tolerance";Result (I,0);" Volts"
420	END IF	
430	! Channel	check
440	OUTPUT	@Mux;"CLOS (@"&Cc\$&"00)"
450	OUTPUT	@Dmm;"TRIG SGL"
460	ENTER @	2Dmm;Result (I,1)
470	IF Result ((I,1) > .01 THEN
480	PRINT	Γ "Channel path leakage out of tolerance";Result (I,1);" Volts"
490	END IF	
500	OUTPUT	@Mux;"*RST"
510	! Tree che	ck
520	OUTPUT	@Mux;"SCAN:PORT ABUS"
530	OUTPUT	@Mux;"CLOS (@"&Cc\$&"00)"
540		@Dmm;"TRIG SGL"
550		Dmm;Result (I,2)
560	•	,2) > .01 THEN
570	PRINT	Γ "Tree A path leakage out of tolerance";Result (I,2);" Volts"

580 END IF

- 590 OUTPUT @Mux;"OPEN (@"&Cc\$&"00)"
- 600 OUTPUT @Mux;"CLOS (@"&Cc\$&"15)"
- 610 OUTPUT @Dmm;"TRIG SGL"
- 620 ENTER @Dmm;Result (I,3)
- 630 IF Result (I,3) > .01 THEN
- 640 PRINT "Tree B path leakage out of tolerance ";Result\$(I,3);" Volts"
- 650 END IF
- 660 OUTPUT @Mux;"*RST"
- 670 IF I < 5 THEN
- 680 PRINT "Test ";I+1;" complete"
- 690 PRINT "Turn power supply OFF"
- 700 PRINT "Press Continue for test ";I+2
- 710 PAUSE
- 720 END IF
- 730 NEXT I
- 740 PRINT "Leakage tests complete"
- 750 DISP "Press Continue to print measurement results"
- 760 PAUSE
- 770 CLEAR SCREEN
- 780 !
- 790 ! Print results
- 800 !
- 810 Format:IMAGE K,3X,D.DDDD," Vdc",3X,D.DDDD," Vdc",3X,D.DDDD, " Vdc",3X,D.DDDD," Vdc"
- 820 PRINT
- 830 PRINT " Positive polarity leakage "
- 840 PRINT " Direct Channels Tree A Tree B"
 - 850 PRINT USING Format;"HI to LO ",Result(0,0),Result(0,1),Result(0,2),Result(0,3)
 - 860 PRINT USING Format;"HI to Chassis ",Result(1,0),Result(1,1),Result(1,2),Result(1,3)
- 870 PRINT USING Format;"LO to Chasis ",Result(2,0),Result(2,1),Result(2,2),Result(2,3)
- 880 PRINT
- 890 PRINT " Negative polarity leakage "
- 900 PRINT " Direct Channels Tree A Tree B"
- 910 PRINT USING Format;"HI to LO ",Result(3,0),Result(3,1),Result(3,2),Result(3,3)
- 920 PRINT USING Format;"HI to Chassis
- ",Result(4,0),Result(4,1),Result(4,2),Result(4,3)
- 930 PRINT USING Format;"LO to Chasis ",Result(5,0),Result(5,1),Result(5,2),Result(5,3)
- 940 END

Typical Result

	Positive polarity	Positive polarity leakage			
	Direct	Channels	Tree A	Tree B	
DIRECT HI to DIRECT LO	0.0021 Vdc	0.0015 Vdc	0.0020 Vdc	0.0018 Vdc	
HI to CHASSIS	0.0019 Vdc	0.0020 Vdc	0.0022 Vdc	0.0022 Vdc	
LO to CHASSIS	0.0015 Vdc	0.0022 Vdc	0.0019 Vdc	0.0023 Vdc	
	Negative polarity leakage				
	Direct	Channels	Tree A	Tree B	
DIRECT HI to DIRECT LO	0.0022 Vdc	0.0026 Vdc	0.0025 Vdc	0.0028 Vdc	
HI to CHASSIS	0.0028 Vdc	0.0030 Vdc	0.0026 Vdc	0.0026 Vdc	
LO to CHASSIS	0.0038 Vdc	0.0033 Vdc	0.0028 Vdc	0.0032 Vdc	

Performance Test Record	Table 2-1, <i>Performance Test Record</i> , is a form you can copy and use to record performance verification test results for the FET Multiplexer. Table 2-1 shows multiplexer test limits, DMM measurement uncertainty, and test accuracy ratio values (TAR).
Test Limits	Test limits are defined for Closed Channel Resistance and Leakage (input isolation) using the specifications in <i>Appendix A</i> of the appropriate <i>User's Manual</i> . The closed channel resistance and leakage tests are single-ended, meaning that there is an upper limit OR a lower limit but not both. In Table 2-1, the minimum or maximum column is blank for a single ended test.
Measurement Uncertainty	For the performance verification tests in this manual, measurement uncertainties are calculated based on the Agilent 3458A Digital Multimeter. The measurement uncertainty shown in Table 2-1 is the accuracy of the Agilent 3458A using 90-day specifications. The calculations follow.
Closed Channel Resistance Test	 Conditions: 2-wire Ohms function, 10 kΩ range 90 day specifications
	• Worst case reading = $3.1 \text{ k}\Omega$ MU = (8 ppm of Reading + 0.5 ppm of Range)
	$= ((8 \times 10^{-6} * 3100) + (0.5 \times 10^{-6} * 10^{4}))$
	$= 0.03 \ \Omega$

Leakage Test Conditions:

- DC Volts function, 100 *m*V range
- 90 day specifications
- Worst case reading = 0.01 V
- Resistor value: 99 k $\Omega < R < 101 \text{ k}\Omega$
- Power supply value: 9.9 Vdc < PS < 10.1 Vdc

3458 Uncert = (5 ppm of Reading + 10 ppm of Range)

=((5 X
$$10^{-6} * 0.01$$
) + (10 X $10^{-6} * 0.1$))

 $= 1.05 \text{ X} 10^{-6} \text{ Volts}$

Resistor Uncert =
$$\left(\frac{10}{10^8 + R_{MAX}} * R_{MAX}\right) - \left(\frac{10}{10^8 + R_{MIN}} * R_{MIN}\right)$$

= $(1.008 X 10^{-2}) - (9.89 X 10^{-3})$
= $1.99 X 10^{-4}$ Volts

Power Supply Uncert =
$$\left(\frac{PS_{MAX}}{1.001 X 10^8} * 10^5\right) - \left(\frac{PS_{MIN}}{1.001 X 10^8} * 10^5\right)$$

= $(1.008 X 10^{-2}) - (9.89 X 10^{-3})$
= $1.99 X 10^{-4}$ Volts

MU = 3458A Uncert + Resistor Uncert + Power Supply Uncert

=
$$(1.05 \times 10^{-6}) + (1.99 \times 10^{-4}) + (1.99 \times 10^{-4})$$

$$= 3.99 \text{ X} 10^{-4} \text{ Volts}$$

Test Accuracy
Ratio (TAR)Test Accuracy Ratios (TAR) are not defined for single-ended
measurements, so all closed channel resistance and leakage current tests
show NA (Not Applicable) in the TAR column.

Table 2-1. Performance Test Record (Page 1 of 2)

Model	Report No	Date
General Information		
Test Facility:		
Name	Report No	
Address	Date	
City/State	Customer	
Phone	Tested by	
Special Notes:		

Test Equipment Record

Test Equipment Used: Description	Model No.	Trace No.	Cal Due Date
1			
2			
3			

Model		Report No	Date		
Test No/Description	Minimum* Value	Measured Value (V)	Maximum Value	Meas Uncert	Test Acc Ratio (TAR)
2-1. Closed Channel Re	esistance (Values	in Ohms)			
Channels		HI LO			
0 1 2 3 4 5 6 7 8 9 10 11			3100 3100 3100 3100 3100 3100 3100 3100	3E-2 3E-2 3E-2 3E-2 3E-2 3E-2 3E-2 3E-2	NA NA NA NA NA NA NA NA NA NA
12 13 14 15 Tree A Tree B			3100 3100 3100 3100 3100 3100 3100	3E-2 3E-2 3E-2 3E-2 3E-2 3E-2	NA NA NA NA NA

Table 2-1. Performance Test Record (Page 2 of 3)

*Single-sided specification - Minimum value does not apply

Model		Report NoDate				
Test No/Description	Minimum Value *	Measured Value (V)	Maximum Value	Meas Uncert	Test Acc Ratio (TAR)	
2-2: Leakage (Values in	Volts)					
Positive polarity						
HI to LO Direct Channels Tree A Tree B			0.01 0.01 0.01 0.01	3.99E-4 3.99E-4 3.99E-4 3.99E-4	NA NA NA NA	
HI to Chassis Direct Channels Tree A Tree B			0.01 0.01 0.01 0.01	3.99E-4 3.99E-4 3.99E-4 3.99E-4	NA NA NA NA	
LO to Chassis Direct Channels Tree A Tree B			0.01 0.01 0.01 0.01	3.99E-4 3.99E-4 3.99E-4 3.99E-4	NA NA NA NA	
Negative polarity						
HI to LO Direct Channels Tree A Tree B			0.01 0.01 0.01 0.01	3.99E-4 3.99E-4 3.99E-4 3.99E-4	NA NA NA NA	
HI to Chassis Direct Channels Tree A Tree B			0.01 0.01 0.01 0.01	3.99E-4 3.99E-4 3.99E-4 3.99E-4	NA NA NA NA	
LO to Chassis Direct Channels Tree A Tree B			0.01 0.01 0.01 0.01	3.99E-4 3.99E-4 3.99E-4 3.99E-4	NA NA NA NA	

Table 2-1. Performance Test Record (Page 3 of 3)

*Single-sided specification - Minimum value does not apply

Introduction	This chapter contains information to order replaceable parts for the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexers. Table 3-1 lists replaceable parts for major assemblies of the FET Multiplexers. Table 3-2 lists selected mechanical parts for the Component assembly. Table 3-3 lists parts for the terminal case. Table 3-4 shows reference designators for the parts listed in Tables 3-1 through 3-3. Table 3-5 shows the manufacturer code list for these parts. To order a part listed in Table 3-1 through through 3-3, specify the Agilent Technologies part number and the quantity required. Send the order to your nearest Agilent Technologies Sales and Support Office.
Replaceable Parts Lists	 Table 3-1 lists the part numbers of the major assemblies of the FET Multiplexers. Table 3-2 lists mechanical replaceable parts for the Component Assembly (common to all FET Multiplexers). Table 3-3 lists replaceable parts for the Terminal Case Assembly (Common to all FET Multiplexers) Figure 3-1 shows the Component Assembly and Figure 3-2 shows the Terminal Case Assembly. A CLIP package, including component level replaceable parts lists, is available for the FET Multiplexers (order Agilent part number
Exchange Assembly	E1351-90033). The component assembly may be replaced on an exchange basis. Exchange assemblies are available only on a trade-in basis. Defective assemblies must be returned for credit. Order assemblies for spare parts stock by the new assembly part number given in Table 3-1. Terminal blocks and case assemblies are not available for exchange. The component assembly exchange part number is: E1351-69201

Table 3-1. FET Multiplexer Replaceable Parts

Reference Designator	Agilent Part Number	Qty	Part Description	Mfr. Code	Mfr. Part Number
			Agilent E1351A		
A1	E1351-66510	1	TERMINAL BLOCK FOR MULTIPLEXER	28480	E1351-66510
A2	E1351-66201	1	16-CHANNEL FET MULTIPLEXER (See Figure 3-1 and Table 3-2)	28480	E1351-66201
A3	E1300-84401	1	CASE ASSEMBLY FOR MULTIPLEXER (See Figure 3-2 and Table 3-3)	28480	E1300-84401
			Agilent E1352A		
A1	E1351-66201	1	16-CHANNEL FET MULTIPLEXER (See Figure 3-1 and Table 3-2)	28480	E1351-66201
A2	E1352-66510	1	TERMINAL CARD 48 C FET MUX	28480	E1352-66510
A4	E1300-84401	1	CASE ASSEMBLY FOR MULTIPLEXER (See Figure 3-2 and Table 3-3)	28480	E1300-84401
			Agilent E1353A		
A1	E1351-66201	1	16-CHANNEL FET MULTIPLEXER (See Figure 3-1 and Table 3-2)	28480	E1351-66201
A2	E1353-66510	1	PC BOARD ASSY; TERMINAL MODULE	28480	E1353-66510
A4	E1300-84401	1	CASE ASSEMBLY FOR MULTIPLEXER (See Figure 3-2 and Table 3-3)	28480	E1300-84401
			Agilent E1357A		
A1	E1355-66510	1	TERMINAL RELAY - 120 OHM FOR MUX	28480	E1355-66510
A2	E1351-66201	1	16-CHANNEL FET MULTIPLEXER (See Figure 3-1 and Table 3-2)	28480	E1351-66201
Α4	E1300-84401	1	CASE ASSEMBLY FOR MULTIPLEXER (See Figure 3-2 and Table 3-3)	28480	E1300-84401
			Agilent E1358A		
A1	E1356-66510	1	TERMINAL RELAY - 350 OHM FOR MUX	28480	E1356-66510
A2	E1351-66201	1	16-CHANNEL FET MULTIPLEXER (See Figure 3-1 and Table 3-2)	28480	E1351-66201
Α4	E1300-84401	1	CASE ASSEMBLY FOR MULTIPLEXER (See Figure 3-2 and Table 3-3)	28480	E1300-84401

Reference Designator	Agilent Part Number	Qty	Part Description	Mfr. Code	Mfr. Part Number
	E1351-66201	1	16-CHANNEL FET MULTIPLEXER	28480	E1351-66201
			(See figure 3-1)		
LBL1	E1300-84308	1	LBL LOGO Agilent B SIZE	28480	E1300-84308
LBL2	E1300-84309	1	LBL LOGO VXI B SIZE	28480	E1300-84309
F1	2110-0712	1	FUSE-SUBMINIATURE 4A 125V NTD AX	75915	R251004T1
F2	2110-0665	1	FUSE-SUBMINIATURE 1A 125V NTD AX UL CSA	75915	R251001T1
J1	1252-1596	2	CONNECTOR-POST TYPE 2.54-PIN-SPCG 96-CONTACT	06776	DIN-96CPC-SRI-TR
J2	1252-3712	1	CONNECTOR-POST TYPE .100-PIN-SPCG 12-CONTACT	18873	68668-004
J3	1252-3868	1	CONNECTOR-POST TYPE .100-PIN-SPCG 6-CONTACT	18873	68668-071
J4	1251-8735	1	CONNECTOR-POST TYPE .100-PIN-SPCG 8-CONTACT	18873	67997-608
MP1-MP2	1400-1546	2	BRACKET PC BOARD HOLDER; BLACK; EXTRUDED	28480	1400-1546
P1	1252-1596		CONNECTOR-POST TYPE 2.54-PIN-SPCG 96-CONTACT	06776	DIN-96CPC- SRI-TR
P4	1258-0247	1	JUMPER-4 POSITIONS HOUSING MATERIAL	18873	69146-204
PNL1	E1351-00202	1	PNL-RR MATRIX SW	28480	E1351-00202
SCR1-SCR2	0515-0444	2	SCREW-MACHINE M2.5 X 0.45 8MM-LG PAN-HD	28480	0515-0444
SCR3-SCR4	0515-1968	2	SCREW PHM 2.5 X 11	28480	0515-1968

Table 3-2. FET Multiplexer Component Assembly Replaceable Parts

Reference Designator	Agilent Part Number	Qty	Part Description	Mfr. Code	Mfr. Part Number
	E1300-84401	1	CASE ASSEMBLY FOR MULTIPLEXER (See Figure 3-2)	28480	E1300-84401
CS1	03852-01201	1	CLAMP	28480	03852-01201
CS2	03852-86701	1	PAD - CLAMP	28480	03852-86701
CS3	0515-2109	1	SCREW - MACHINE 10-24 .625-IN-LG PAN-HD-SLT	28480	0515-2109
CS4	1390-0846	2	FASTENER-CAPTIVE SCREW M2.5 X 1.45 THREAD	28480	1390-0846
CS5	E1300-01202	1	CLAMP-STRAIN RELEIF	28480	E1300-01202
CS6	E1300-44101	1	COVER-TOP, TERMINAL HOUSING, MOLDED	28480	E1300-44101
CS7	E1300-44102	1	COVER-BOTTOM, TERMINAL HOUSING	28480	E1300-44102

Table 3-3. Terminal Case Replaceable Parts

Table 3-4. FET Multiplexers Reference Designators

FET Multiplexers Reference Designators								
	MP mechanical part							
LBLlabel	Pelectrical connector (plug)							
	PNLpanel							
J electrical connector (jack)	SCR screw							
JMjumper	SWswitch							

Table 3-5. FET Multiplexer Code List of Manufacturers

Mfr. Code	Manufacturer's Name	Manufacturer's Address	Zip Code
06776	ROBINSON NUGENT INC	NEW ALBANY NY US	47150
18873	DUPONT E I DE NEMOURS & CO	WILMINGTON DE US	19801
26742	METHODE ELECTRONICS INC	CHICAGO IL US	60656
28480	AGILENT TECHNOLOGIES - CORPORATE	PALO ALTO CA US	94304
75915	LITTELFUSE INC	DES PLAINES IL US	60016
76381	ЗМ СО	ST PAUL MN US	55144
81073	GRAYHILL INC	LA GRANGE IL US	60525

Mechanical Parts Locators

Figure 3-1 shows the mechanical replaceable parts on the component assembly (Agilent PN E1351-66201). Figure 3-2 shows the mechanical replaceable parts for the terminal case assembly (Agilent PN E1300-84401).

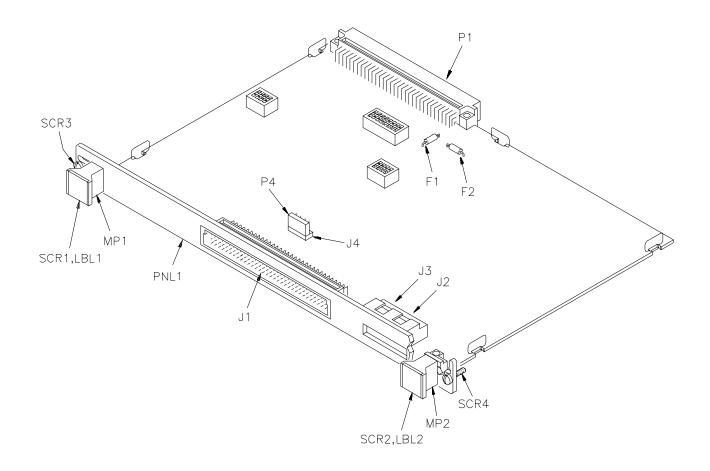


Figure 3-1. Component Assembly Replaceable Parts

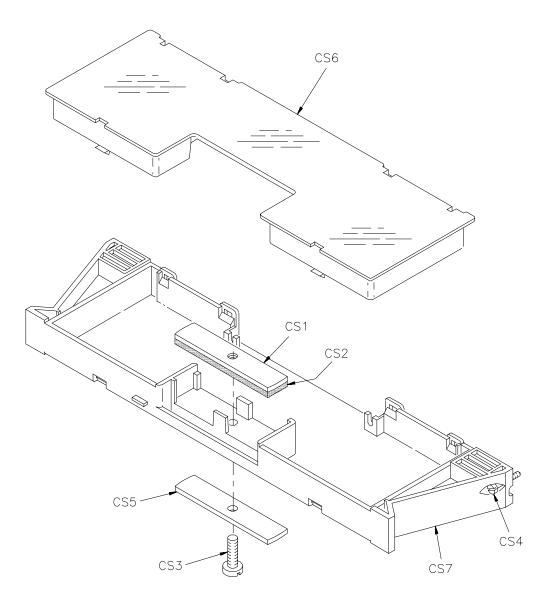


Figure 3-2. Terminal Case Assembly Replaceable Parts

Introduction	This chapter contains service information for the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexers. Also included are trouble shooting, repair, and maintenance guidelines. Do not perform any of the service procedures shown unless you are a qualified, service-trained technician and have read the WARNINGS and CAUTIONS in Chapter 1.		
WARNING			
Equipment Required	Equipment required for module troubleshooting and repair is listed in <i>Table 1-1, Recommended Test Equipment</i> . Any equipment that satisfies the requirements given in the table may be substituted. To avoid damage to the screw head slots, use a T8 Torx driver to remove the front panel handles.		
Service Aids	See <i>Chapter 3</i> — <i>Replaceable Parts</i> for descriptions and locations of Agilent E1351A, E1352A, E1353A, E1357A, and E1358A replaceable parts. Service notes, manual updates, and service literature for the FET Multiplexers may be available through Agilent Technologies. For information, contact your nearest Agilent Technologies Sales and Service Office.		
FET Multiplexer Description	The Agilent E1351A, E1352A, E1353A, E1357A, and E1358A all use a common component assembly. The component assembly contains all the FET switches and their associated protection circuitry. Each terminal block configures the component assembly to the appropriate type of switch. Figures 4-1 through 4-4 show a simplified switching diagram for each FET Multiplexer.		
	The terminal card contains the model identification code and the installation of the terminal card before applying mainframe power ensures that the type of switch is correctly identified. Optionally, the model identification can be set on the component assembly to allow it to be correctly identified without a terminal card installed. The component module also contains jumpers that place the internal +4.6 V strain gage excitation voltage on the terminal block		

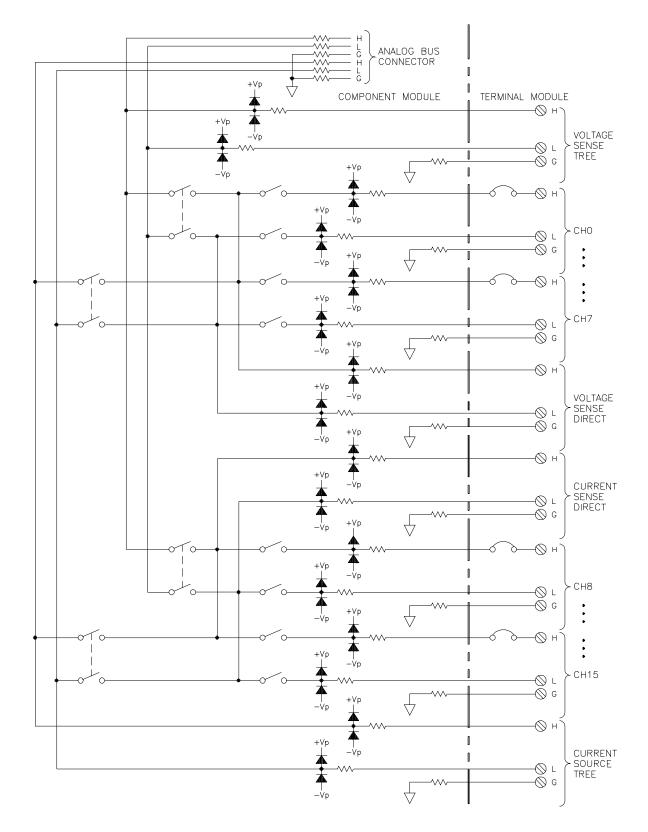
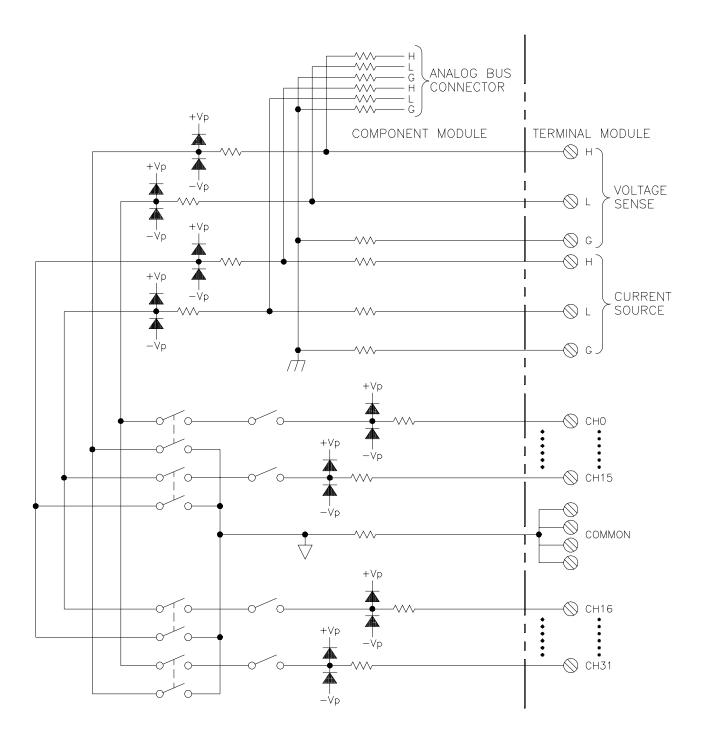


Figure 4-1. Agilent E1351A Simplified Switch Diagram





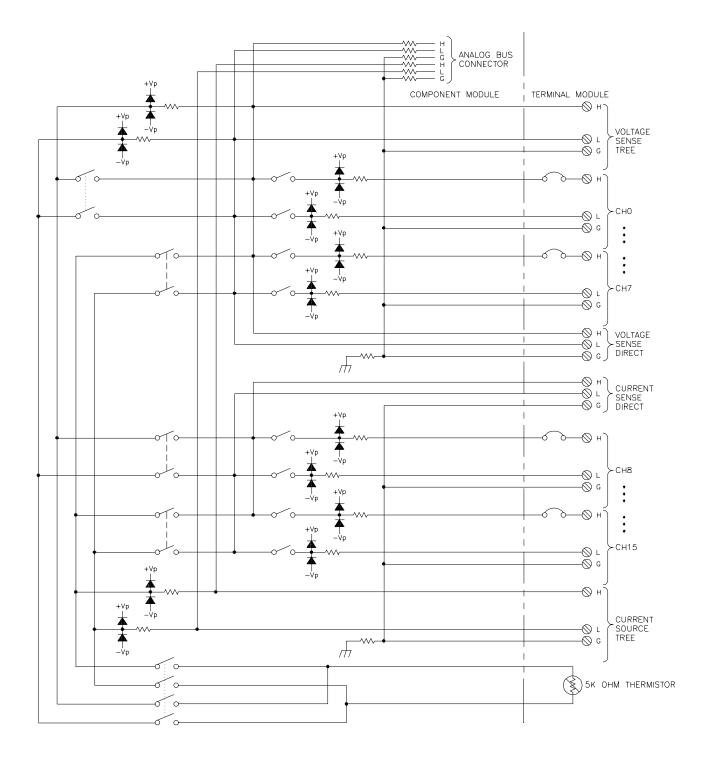


Figure 4-3. Agilent E1353A Simplified Switch Diagram

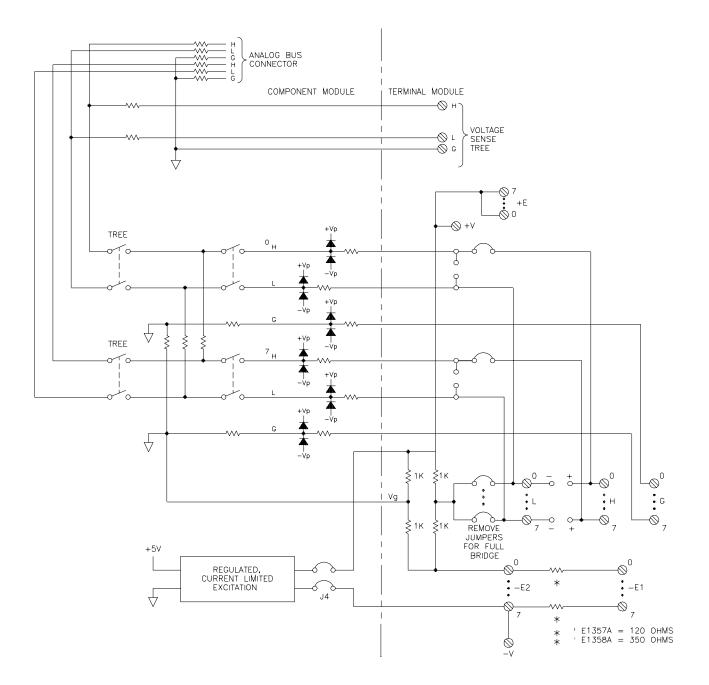


Figure 4-4. Agilent E1357A/58A Simplified Switch Diagram

	for use with the Agilent E1357A and Agilent E1358A Strain Gage FET Multiplexers.		
Repair Strategy	Agilent Technologies recommends replacement of the entire assembly in the event of a failure. Procedures in this chapter describe troubleshooting techniques. A CLIP package, including component level replaceable parts lists, is available for the FET Multiplexers (order Agilent part number E1351-90033). The component assembly is available as an exchange asembly as described in <i>Chapter 3</i> — <i>Replaceable Parts</i> . Be sure to perform the tests and checks in Table 4-2 before exchanging an assembly.		
Troubleshooting Techniques	To troubleshoot a FET Multiplexer problem you must first identify the problem and then isolate the cause of the problem to a replaceable assembly. See <i>Chapter 3</i> — <i>Replaceable Parts</i> for descriptions and locations of Agilent E1351A, E1352A, E1353A, E1357A, and E1358A replaceable parts.		
Identifying the Problem	Table 4-1 lists some common problems for the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexers, along with symptoms and possible solutions. If the problem cannot be identified using these steps, replace the assembly.		

Symptom	Recommended Action		
Non-zero error code in response to SYST:ERR?	See Appendix A of the appropriate FET Multiplexer User's Manual.		
Module not responding to commands.	See "Making Visual Checks" in this chapter		
Module fails Closed Channel Resistance Test (Test 2-1) or Leakage Test (Test 2-2)	See "Testing the Module" in this chapter		

Table 4-1. FET Multiplexer Typical Problems

Making Visual Checks	Visual checks for the FET Multiplexers include the following. See Table 4-2 for typical checks.		
	Check switches/jumpersCheck for heat damageChecking connector contacts		
NOTE	See the appropriate FET Multiplexer User's Manual for information or		

See the appropriate FET Multiplexer User's Manual for information on logical address and IRQ settings. If there are no apparent problems following the visual checks, run the Performance Verification Tests in Chapter 2 to see if the module is defective.

Test/Check	Reference Designator	Check	Action/Notes
Heat Damage		Discolored PC boards Damaged insulation Evidence of arcing	If there is damage, do not operate the module until you have corrected the problem.
Switch/Jumper Settings	SP2 SP1 SP3 J4 JM1	IRQ Level setting Logical address setting Card ID Strain Excitation Remote Ground Sense	Factory set at 1 Factory set at 112 Factory set 00 Factory set to OFF Factory Installed
Component Assembly	F1, F2 J1, J2, J3 P1	Fuse continuity Dirty or bent connector pins Dirty or bent connector pins	Check fuses with ohmmeter Straighten/clean pins Straighten/clean pins

Table 4-2. FET Multiplexer Visual Tests/Checks

Testing the Module

You can use the tests and checks in *Chapter 2*—*Verification Tests* to identify a problem with the assembly. See *Chapter 3*—*Replaceable Parts* for locations of mechanical parts.

Repair and Maintenance Guidelines	 This section provides guidelines for repairing and maintaining the FET Multiplexer including: ESD precautions Soldering printed circuit boards Post-repair safety checks
ESD Precautions	Electrostatic discharge (ESD) may damage static sensitive devices in the module. This damage can range from slight parameter degradation to catastrophic failure. When handling the module observe the following guidelines:
	• Always use a static-free work station with a pad of conductive rubber or similar material when handling module components.
	• If a device requires soldering, be sure the assembly is placed on a pad of conductive material. Also, be sure that you, the pad, and the soldering iron tip are grounded to the assembly.
Soldering Printed Circuit Boards	The etched circuit board of this module has plated-through holes that provide a solder path to both sides of the insulating material. Soldering can be done from either side of the board with equally good results. When soldering to any circuit board, keep in mind the following guidelines:
	• Avoid unnecessary component unsoldering and soldering. Excessive replacement can result in damage to the circuit board, adjacent components, or both.
	• Do not use a high power soldering iron on etched circuit boards, as excessive heat may lift a conductor or damage the board.
	• Use a suction device or wooden toothpick to remove solder from component mounting holes. When using a suction device, be sure that the equipment is properly grounded.
Post-Repair Safety Checks	After making repairs to the module, inspect the module for any signs of abnormal internally generated heat, such as discolored printed circuit boards or components, damaged insulation, or evidence of arcing. Determine and correct the cause of the condition. Then perform Test 2-1 as described in <i>Chapter 2 — Verification Tests</i> to verify that the module is functional.

Chapter A Verification Tests - C Programs

Functional Verification Test	This program is designed to do the Functional Verification Test found in <i>Chapter 2 - Verification Tests</i> .		
Example: Self Test	The Functional Verification Test for the Agilent E1351A, E1352A, E1353A, E1357A, and E1358A FET Multiplexers consists of sending the *IDN? command and checking the response. This test can be used to verify that the FET Multiplexer is connected properly and is responding to a basic command.		
NOTE	This program assumes a primary address of 09 and a secondary address of 14. If your FET Multiplexer address does not match this, you must either change the FET Multiplexer address setting or change the program line #define ADDR "hpib7,9,14" to match your FET Multiplexers address setting.		
#incl #def	ude <stdio.h> ude <sicl.h> ine ADDR "hpib7,9,14" main (void)</sicl.h></stdio.h>	/* Address of device */	
	BT id; ir a[256] = {0};	/* Define id as an instrument */ /* Result variable */	
ion id =	error (I_ERROR_EXIT); iopen (ADDR);	/* Open instrument session */	
isca prir get	ntf(id, "*IDN?\n"); anf (id, "%t", a); itf("\n %s", a); char(); se (id);	/* Send *IDN? command */ /* Get response */ /* Print result */ /* Pause */ /* Close instrument session */	

Performar Verificatio Tests		These programs are designed to do the Performance Verification Tests found in <i>Chapter 2 - Verification Tests</i> .		
NOTE		These programs assume a primary address of 09 and a secondary address of 14. If your FET Multiplexer address does not match this, you must either change the FET Multiplexer address setting or change the program lines #define ADDR "hpib7,9,14" to match your FET Multiplexers address setting.		
Example: (Resistar	Channel	This example performs a closed channel resistance test of all measurement paths. If a FET on resistance is >3.1 k Ω , the program prints a message indicating which channel has failed. Before the closed channel measurement, the program checks for stuck channels. If a stuck channel is found, the program prints a message and halts.		
	/* Clos	sed-channel Resistance Test E1351A */		
		de <stdio.h> de <sicl.h></sicl.h></stdio.h>		
	#define #define	e ADDR "hpib7,9,14" /* Address of device */ e DMM "hpib7,22"		
	void m	ain (void)		
	int i, j doub char	id, dm; /* Define id and dm as an instrument */ ; le result[2][15], tree[2][2], value; cr[256]; *path;		
		fined(BORLANDC) && !defined(WIN32) EasyWin(); if		
	dm =	ror(I_ERROR_EXIT); iopen (DMM); /* Open instrument session */ open(ADDR);		
	printf printf printf printf printf	("\n\n\nInstall Component Assembly and Test Fixture"); ("\n\n 1. Turn Mainframe AND 3458a DMM power OFF."); ("\n 2. Connect GPIB Cable between mainframe and DMM."); ("\n 3. Install Agilent E1351A Component Assembly into Mainframe."); ("\n 4. Attach Test Fixture to Component Assembly."); ("\n 5. Turn Mainframe and DMM power ON"); ("\n 6. Press ENTER when ready to begin testing."); mar ();		

```
/*......Measure Closed Channel Resistance......*/
 iprintf (id. "*RST\n"):
 iprintf (dm, "PRESET NORM;TRIG HOLD\n");
 iprintf (dm, "END ALWAYS\n");
 iprintf (dm, "FUNC OHM\n");
 for (i = 0; i \le 1; i++)
 ł
  if (i == 0) path = "HI";
             \dot{p}ath = "LO";
  else
  printf ("\n\nChannel %s to Direct %s Measurements", path, path);
  printf ("\n\n 1. Connect DMM Input HI lead to Channel %s", path);
  printf ("\n 2. Connect DMM Input LO lead to Direct %s", path);
  printf ("\n 3. Press ENTER when connections are complete");
  getchar ();
  /*-----Check for stuck channels-----*/
  iprintf (id, "*RST\n");
  iprintf (dm, "TRIG SGL\n");
iscanf (dm, "%lf", &value);
iscanf (dm, "%t", cr);
  if (value < 10000)
  ł
    printf ("\n\n**** Measurement indicates a stuck channel *****");
printf ("\n**** Correct the problem before proceeding *****");
   goto EXIT;
  for (j = 0; j \le 15; j++)
    iprintf (dm, "TRIG SGL\n");
iscanf (dm, "%lf", &result[i][j]);
iscanf (dm, "%t", cr);
printf ("\nchannel %u resistace = %6.4lf", j, result[i][j]);
    if (j < 10) iprintf (id, "OPEN (@10%u)\n", j);
                iprintf (id, "OPEN (@1%u)\n", j);
    else
    if (result[i][j] > 3100) printf ("\n*** Resistance for Channel %u is 3.1 kOhms ***
%6.4lf Ohms", j, result[i][j]);
  if (i == 0)
    printf ("\n\nMeasurements complete for channel HI.");
    printf ("\nPress ENTER for channel LO measurements");
    getchar ();
  }
  else
    printf ("\n\nMeasurements complete for channel LO.");
  }
 }
```

```
printf ("\n\nMeasurements complete for Channel HI and LO");
printf ("\nPress ENTER for Tree Switch measurements");
getchar ();
/*......Tree Switch Measurements......*/
iprintf (dm, "PRESET NORM;TRIG HOLD\n");
iprintf (dm, "END ALWAYS\n");
iprintf (dm, "FUNC OHM\n");
for (i = 0; i \le 1; i++)
ł
 if (i == 0)
  ł
   path = "HI";
   printf ("\n\nTree HI to Direct HI Measurements");
printf ("\n\n 1. Connect DMM Input HI leads to Tree HI");
   printf ("\n 2. Connect DMM Input LO leads to Direct HI");
  else
   path = "LO":
   printf ("\n\nTree LO to Direct LO Measurements");
   printf ("\n\n 1. Connect DMM Input HI leads to Tree LO");
   printf ("\n 2. Connect DMM Input LO leads to Direct LO");
 printf ("\n 3. Press ENTER when connections are complete.");
 getchar ();
 iprintf (id, "*RST\n");
 /*-----Check for stuck channels-----*/
 iprintf (dm, "TRIG SGL\n");
iscanf (dm, "%lf", &value);
iscanf (dm, "%t", cr);
 if (value < 10000)
 ł
   printf ("\n\n***** Measurement indicates a stuck channel *****");
printf ("\n***** Correct the problem before proceeding *****");
   goto EXIT;
 }
 for (j = 0; j <= 1; j++)
   iprintf (id, "SCAN:PORT ABUS\n");
   if (j == 0) iprintf (id, "CLOS (@100)\n");
else iprintf (id, "CLOS (@115)\n");
```

```
if (tree[i][j] > 3100)
      if (j == 0) printf ("\n*** Resistance for A Tree Switch is 3.1 kOhms");
else printf ("\n*** Resistance for B Tree Switch is 3.1 kOhms");
    }
   }
   if (i == 0)
    printf ("\n\nMeasurements complete for Tree Switch HI");
printf ("\nPress ENTER forTree Switch LO measurements");
    getchar();
   }
   else
   {
    printf ("\n\nMeasurements complete for Tree Switch LO");
   }
 }
 printf ("\n\nClosed channel resistance measurements complete.");
printf ("\nPress ENTER to display measurement results.");
 getchar ();
 /*.....Display Measurement Results.........................*/
 printf ("\n\n-----");
printf ("\n\nClosed Channel Resistance measurement Results\n");
 for (j = 0;j <= 15; j++)
   printf ("\n Channel %u HI = %6.4lf Ohms LO = %6.4lf Ohms", j+100,
result[0][j], result[1][j]);
 }
 printf ("\n\n Tree A
                              HI = %6.4lf Ohms LO = %6.4lf Ohms", tree[0][0],
tree[1][0]);
 printf ("\n Tree B
                           HI = %6.4lf Ohms LO = %6.4lf Ohms", tree[0][1], tree[1][1]);
EXIT:
 iclose (id); iclose (dm);
                                                         /* Close instrument session */
}
```

Example: Leakage Current Test

This example performs a leakage test from HI to LO, HI to Chassis, and LO to Chassis. If the leakage is too high (caused by a failure of the input impedance), the test prints a message indicating which leakage path has failed and halts.

/* Leakage Current Test	E1351A */			
#include <stdio.h> #include <sicl.h></sicl.h></stdio.h>				
#define ADDR "hpib7,9,14" #define DMM "hpib7,22"	/* Address of device */			
void main (void)				
{ INST id, dm; int i; double result[6][4], value; char cr[256]; char *path;	/* Define id and dm as an instrument *,			
#if defined(BORLANDC) _InitEasyWin(); #endif	&& !defined(WIN32)			
ionerror(I_ERROR_EXIT);				
dm = iopen (DMM); id = iopen(ADDR);				
itimeout (dm, 10000); itimeout (id, 10000);				
printf ("\n\n 1. Turn Mainframe printf ("\n 2. Connect GPIB Ca	Ind DMM power ON");			
/*Measure Le	eakage*/			
iprintf (dm, "PRESET NORM;TRIG HOLD\n"); iprintf (dm, "END ALWAYS\n"); iprintf (dm, "FUNC DCV\n");				
for (i = 0;i <= 5; i++)				
{ iprintf (id, "*RST\n");				

```
if (i == 0)
   ł
     printf ("\n2. Connect DMM input HI leads to Power Supply HI");
printf ("\n3. Connect DMM input LO leads to Direct HI");
printf ("\n4. Connect Power Supply LO to Direct LO");
   if (i == 1)
     printf ("\n2. Connect DMM input HI leads to Direct HI");
     printf ("\n3. Connect DMM input LO leads to Power Supply LO");
     printf ("\n4. Connect Power Supply HI to Direct LO");
   if (i == 2)
   ł
     printf ("\n2. Connect DMM input HI leads to Power Supply HI");
printf ("\n3. Connect DMM input LO leads to Direct LO");
     printf ("\n4. Connect Power Supply LO to Chassis");
   if (i = 3)
     printf ("\n2. Connect DMM input HI leads to Direct HI");
printf ("\n3. Connect DMM input LO leads to Power Supply LO");
     printf ("\n4. Connect Power Supply HI to Chassis");
   if (i == 4)
    ł
     printf ("\n2. Connect DMM input HI leads to Power Supply HI");
     printf ("\n3. Connect DMM input LO leads to Direct LO");
     printf ("\n4. Connect Power Supply LO to Chassis");
   if (i == 5)
   {
    printf ("\n2. Connect DMM input HI leads to Direct LO");
printf ("\n3. Connect DMM input LO leads to Power Supply LO");
printf ("\n4. Connect Power Supply HI to Chassis");
   printf ("\n5. Turn ON power supply and set output for +10 Vdc");
   printf ("\n6. Press ENTER when connections are complete");
   getchar ();
   printf (".");
iprintf (dm, "TRIG SGL\n");
iscanf (dm, "%lf", &result[i][0]);
iscanf (dm, "%t", cr);
   if (result[i][0] > .01)
printf ("\n\n**** Direct path leakage out of tolerance %6.4lf Volts *****",
result[i][0]);
   /*.....Channel Check.....*/
   printf (".");
iprintf (id, "CLOS (@100)\n");
   iprintf (dm, "TRIG SGL\n");
iscanf (dm, "%lf", &result[i][1]);
iscanf (dm, "%t", cr);
```

```
if (result[i][1] > .01)
    printf ("\n\n***** Channel path leakage out of tolerance %6.4lf Volts *****",
result[i][1]);
   /*.....Tree Check.....*/
  printf (".");
iprintf (id, "SCAN:PORT ABUS\n");
iprintf (id, "CLOS (@100)\n");
iprintf (dm, "TRIG SGL\n");
iscanf (dm, "%lf", &result[i][2]);
iscanf (dm, "%t", cr);
   if (result[i][2] > .01)
    printf ("\n\n***** Tree A path leakage out of tolerance %6.4lf Volts *****",
result[i][2]);
  printf (".");
iprintf (id, "OPEN (@100)\n");
iprintf (id, "CLOS (@115)\n");
iprintf (dm, "TRIG SGL\n");
iscanf (dm, "%lf", &result[i][3]);
iscanf (dm, "%t", cr);
   if (result[i][3] > .01)
    printf ("\n\n***** Tree B path leakage out of tolerance %6.4lf Volts *****",
result[i][3]);
   printf (".");
   if (i < 5)
   ł
    printf ("\n\nTest %u complete", i+1);
printf ("\nTurn power supply OFF");
     printf ("\nPress ENTER for test %u", i+2);
    getchar ();
   }
 3
 printf ("\n\nLeakage tests complete.");
printf ("\nPress ENTER to display measurement results.");
 getchar ();
 /*.....Display Measurement Results.....*/
 printf ("\n\n---
                                                                         -----");
 printf ("\n
printf ("\n---
printf ("\n
                                                                        \n");
-----");
                               Positive Polarity Leakage
                             -----
                           Direct
                                        Channels Tree A
                                                                        Tree B\n");
                                %6.4lf Vdc %6.4lf Vdc %6.4lf Vdc %6.4lf Vdc", result[0][0],
 printf ("\nHI to LO
result[0][1], result[0][2], result[0][3]);
printf ("\nHI to Chassis %6.4lf Vdc %6.4lf Vdc %6.4lf Vdc %6.4lf Vdc ",
result[1][0], result[1][1], result[1][2], result[1][3]);
printf ("\nLO to Chassis %6.4lf Vdc %6.4lf Vdc %6.4lf Vdc %6.4lf Vdc ",
result[2][0], result[2][1], result[2][2], result[2][3]);
```

printf ("\n\n				");
printf ("\n printf ("\n	Negative Polarity Leakage \n");			
printf ("\n	Direct	Channels	Tree A	Tree B\n");
result[3][1], resul printf ("\nHI to (result[4][0], resul	lt[3][2], resul Chassis %6 lt[4][1], resul Chassis %6	lt[3][3]); .4lf Vdc %6 lt[4][2], resul 5.4lf Vdc %	6.4lf Vdc % lt[4][3]); 6.4lf Vdc	5.4lf Vdc %6.4lf Vdc", result[3][0], %6.4lf Vdc %6.4lf Vdc", %6.4lf Vdc %6.4lf Vdc",
iclose (id);iclose }	e (dm);		/* Clo	se instrument session */