


# Agilent E1508A

## 8-Channel x16 Gain & 7 Hz Fixed Filter SCP

### Data Sheet

- Use with Agilent E1413C/E1415A/E1419A
- x16 amplifier and fixed 7 Hz filter
- $\pm 1$  V maximum input with over-voltage protection
- Open transducer detection

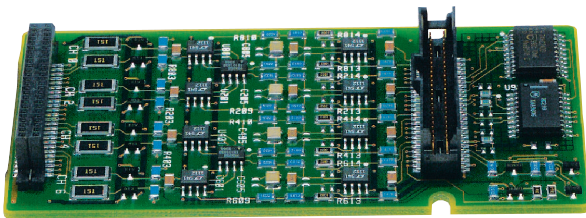

Agilent E1508A

## Description

The Agilent E1508A 8-Channel x16 Gain & 7 Hz Fixed Filter SCP provides eight fixed, 2-pole, low-pass filters with a 3 dB cutoff frequency of 7 Hz and eight amplifiers with a gain of 16. It also provides input over-voltage protection and open transducer detection on each channel.

Use the E1508A with the following VXI modules:

Model	Description
E1413C	64-Channel Scanning A/D Converter
E1415A	Algorithmic Closed Loop Controller
E1419A	Multifunction Measurement and Control Module

Refer to the Agilent Technologies Website for recent product updates, if applicable.

## Voltage Measurements

The E1508A is ideal for measuring signals from sensors with full-scale voltage outputs from 3.9 mV to 1 V. The 2-pole, low-pass filter reduces sensor-based noise in the measurement.

## Temperature Measurements

The E1508A can be used to make temperature measurements with thermocouples, thermistors, or RTDs. Temperature measurements with thermistors or RTDs require the E1505A 8-Channel Current Source SCP. Engineering units conversion to degrees C are made at full speed.



## Resistance Measurements

Resistance is measured using the E1505A 8-Channel Current Source SCP with the E1508A SCP. Measurements are made by applying a dc current to the unknown resistance and measuring the voltage drop across the unknown resistance. The current source is provided through the E1505A. The recommended application is as shown here using 4-wire  $\Omega$  connections. Two-wire  $\Omega$  measurements are possible but not recommended since two 150  $\Omega$  series resistors protecting the input FET multiplexer are included in the measurement.

## Strain Measurements

The E1508A can be used to make strain measurements when combined with either the E1506A or 1507A Strain Completion SCPs. Refer to the E1506A/E1507A *Technical Specifications* for more information.

## Product Specifications

These specifications for the E1508A reflect the combined performance of the scanning A/D and the E1508A SCP.

### Measurement Ranges

<b>DC Volts:</b>	$\pm 3.9$ mV to $\pm 1$ V Full Scale
<b>Temperature:</b>	
<b>Thermocouples:</b>	-200 to + 1700 °C
<b>Thermistors: *</b>	-80 to + 160 °C
<b>RTD's: *</b>	-200 to + 850 °C
<b>Resistance: **</b>	8 $\Omega$ to 32.7 k $\Omega$
<b>Strain: **</b>	25,000 $\mu\epsilon$ or limit of linear range of strain gage

\*Requires Agilent E1505A.

\*\*Requires Agilent E1506A/E1507A.

### Input Characteristics

**Maximum input voltage (normal mode plus common mode):**

<b>Operating:</b>	$< \pm 16$ V peak
<b>Damage level:</b>	$> \pm 42$ V peak

**Maximum common mode voltage:**

<b>Operating:</b>	$< \pm 16$ V peak
<b>Damage level:</b>	$> \pm 42$ V peak

**Input Impedance:** Greater than 100 M $\Omega$  differential

### Maximum Tare Cal Offset

Maximum tare cal offset depends on A/D range and SCP gain.

A/D Range $\pm$ V F. Scale	Maximum Offset
16	0.20009
4	0.05007
1	0.01317
0.25	0.00349
0.0625	0.00112

### Measurement Accuracy DC Volts

If autoranging is ON, add  $\pm .02\%$  FS to accuracy specifications.

Fixed Gain x16 Range $\pm$ V FS	Linearity % of Reading	Offset Error	Noise 3 $\sigma$	Noise* 3 $\sigma$
.0039	0.01%	3.8 $\mu$ V	3.4 $\mu$ V	2.9 $\mu$ V
.0156	0.01%	4.2 $\mu$ V	4.4 $\mu$ V	3.8 $\mu$ V
.0625	0.01%	4.9 $\mu$ V	7.5 $\mu$ V	6.3 $\mu$ V
.256	0.01%	8 $\mu$ V	28 $\mu$ V	23 $\mu$ V
1.0	0.01%	31 $\mu$ V	113 $\mu$ V	64 $\mu$ V

\* A/D filter ON (min sample period  $\geq 145$   $\mu$ s:  $\leq 100$  Hz scan rate 64 ch).

### Temperature Coefficients:

	Temp Range	Tempco
<b>Gain:</b>		15 ppm/°C
<b>Offset:</b>	0-30 °C	0.16 $\mu$ V/°C
	30-40 °C	0.18 $\mu$ V/°C
	40-55 °C	0.39 $\mu$ V/°C

### Normal Mode Rejection

<b>10 Hz LP filter:</b>	
10 Hz:	-6 dB
50 Hz:	$> -23$ dB
60 Hz:	$> -25$ dB

### Common Mode Rejection

<b>0 to 60 Hz:</b>	
Typical:	$> -108$ dB
Minimum:	$> -100$ dB

## Temperature Measurement Accuracy

The thermocouple graphs following this description include the errors due to measuring the voltage output of the thermocouple, and the algorithm errors due to converting the thermocouple voltage to temperature or the Measurement/Conversion Error (MCE). To this error the Reference

Junction Measurement Error (RJME) must be added due to measuring the reference junction temperature with an RTD or thermistor (this measurement requires an E1505A). Also, the Isothermal Reference Gradient Errors (IRGE) must be added due to gradients across the isothermal reference. If an external isothermal reference panel is used, consult the manufacturer's specifications. If Agilent terminal blocks are used as the isothermal reference, see the notes below.

$$\text{Total Temperature Error} = [ (\text{MCE})^2 + (\text{RJME})^2 + (\text{IRGE})^2 ]^{1/2}$$

### NOTES:

1) When using the Terminal Block as the isothermal reference, add  $\pm 0.6^\circ\text{C}$  to the thermocouple accuracy specs to account for temperature gradients across the Terminal Block. The ambient temperature of the air surrounding the Terminal Block must be within  $\pm 2^\circ\text{C}$  of the temperature of the inlet cooling air to the VXI mainframe.




2) When using the Agilent E1586A Rack Mount Terminal Panel as the isothermal reference, add  $\pm 0.2^\circ\text{C}$  to the thermocouple accuracy specs to account for temperature gradients across the E1586A. The E1586A should be mounted in the bottom part of the rack, below and away from other heat sources, for best performance.







All specifications for the following were measured with the A/D filter off.







The following temperature accuracy graphs include instrument and firmware linearization errors. The linearization algorithm used is based on the ITS-90 transducer curves. Add your transducer accuracy to determine total measurement error.







### Conversion Chart






Opt 011	=	E1501A
Opt 012	=	E1502A
Opt 013	=	E1503A
Opt 015	=	E1505A
Opt 016	=	E1506A
Opt 017	=	E1507A
Opt 018	=	E1508A
Opt 019	=	E1509A
Opt 020	=	E1510A
Opt 021	=	E1511A

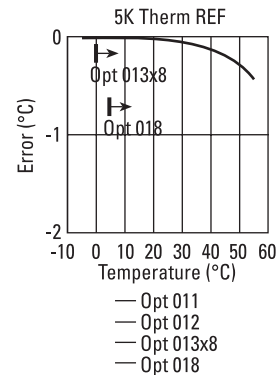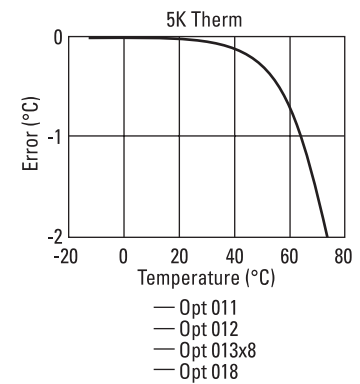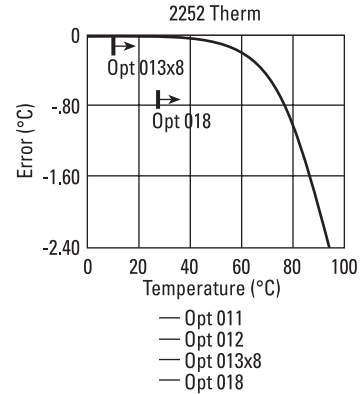

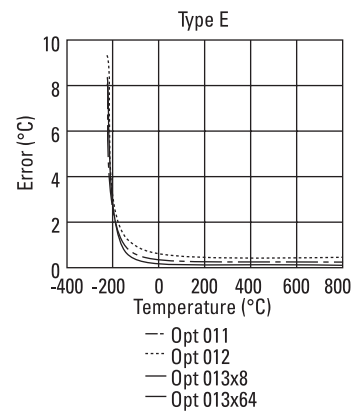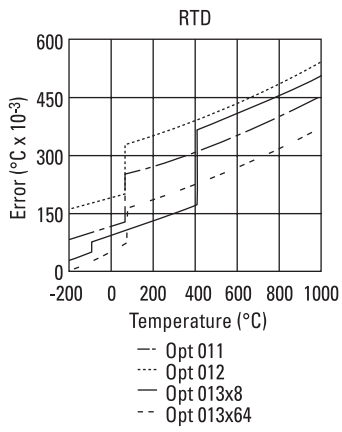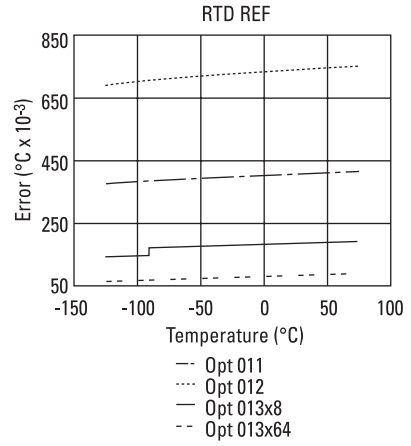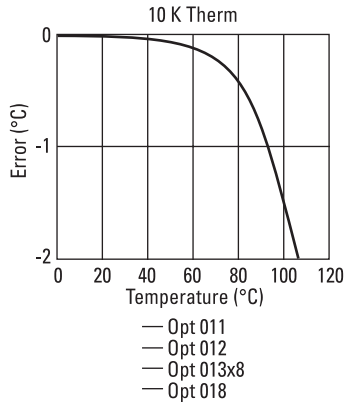

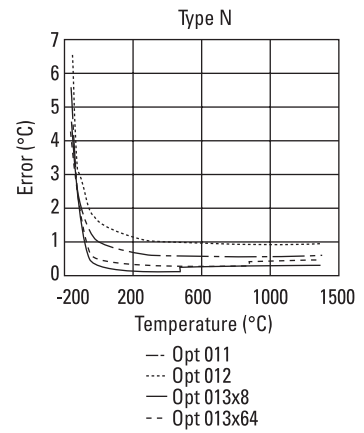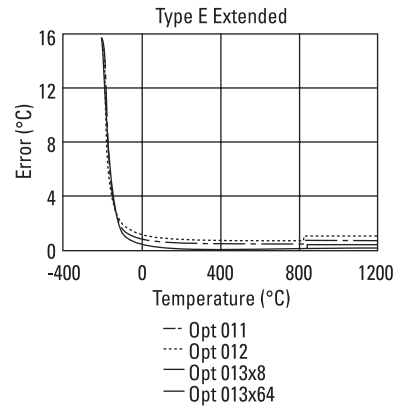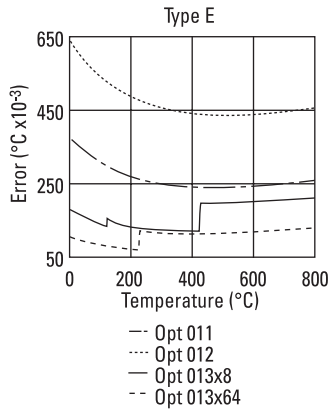

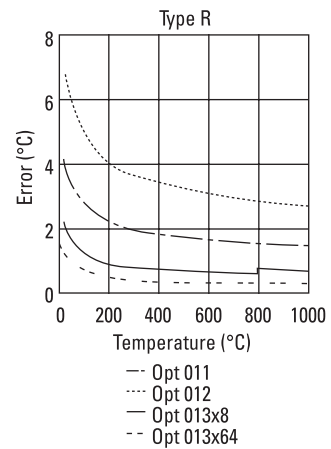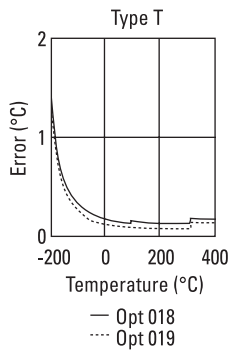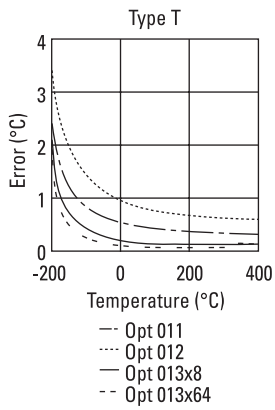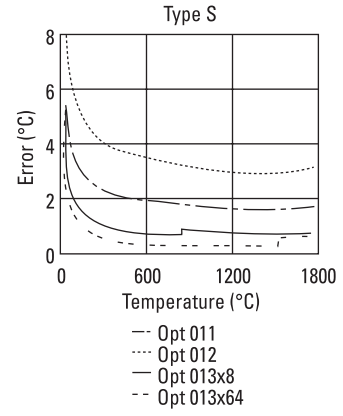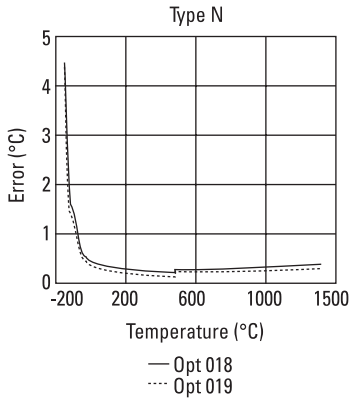

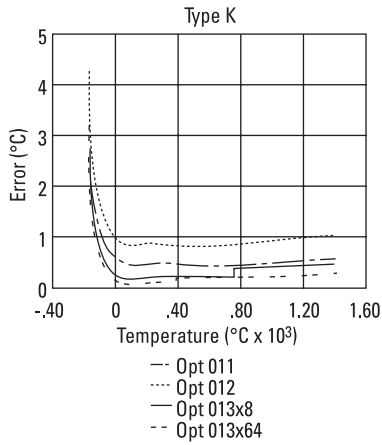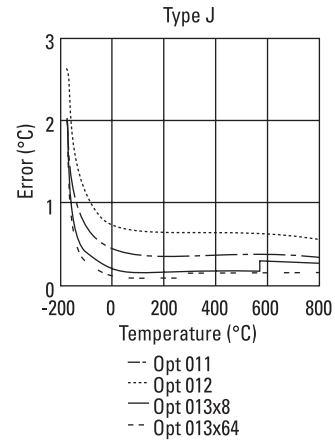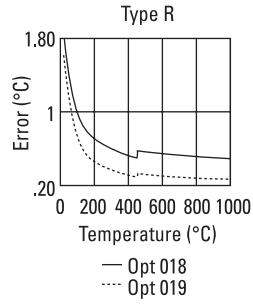


---

**Current Requirements (Amps)**

5 V max	24 V max	-24 V max
0.01	0.02	0.02

---



---

**Ordering Information**

Description	Product No.
8-Channel x16 Gain & 7 Hz Fixed Filter SCP	E1508A

## Related Literature

*2000 Test System and VXI Catalog CD-ROM*,  
Agilent Pub. No. 5980-0308E (detailed specifications for VXI products)

*2000 Test System and VXI Catalog*,  
Agilent Pub. No. 5980-0307E (overview of VXI products )

*1998 Test System and VXI Products Data Book*,  
Agilent Pub. No. 5966-2812E

## Online

Internet access for Agilent product information, services and support  
[www.agilent.com/find/tmdir](http://www.agilent.com/find/tmdir)

VXI product information  
[www.agilent.com/find/vxi](http://www.agilent.com/find/vxi)

Defense Electronics Applications  
[www.agilent.com/find/defense\\_ATE](http://www.agilent.com/find/defense_ATE)

Agilent Technologies VXI Channel Partners  
[www.agilent.com/find/vxichanpart](http://www.agilent.com/find/vxichanpart)

Agilent Technologies' HP VEE Application Website  
[www.agilent.com/find/vee](http://www.agilent.com/find/vee)

Agilent Technologies Data Acquisition and Control Website  
[www.agilent.com/find/data\\_acq](http://www.agilent.com/find/data_acq)

Agilent Technologies Instrument Driver Downloads  
[www.agilent.com/find/inst\\_drivers](http://www.agilent.com/find/inst_drivers)

Agilent Technologies Electronics Manufacturing Test Solutions  
[www.agilent.com/go/manufacturing](http://www.agilent.com/go/manufacturing)

**Get assistance with all your test and measurement needs at  
[www.agilent.com/find/assist](http://www.agilent.com/find/assist)  
or check your local phone book for the Agilent office  
near you.**

## Agilent Technologies' test and measurement service/support commitment

Agilent strives to maximize the value our test and measurement products give you, while minimizing your risk and service/support problems. We work to ensure that each product is realistically described in the literature, meets its stated performance and functionality, has a clearly stated global warranty, and is supported at least five years beyond its production life. Our extensive self-help tools include many online resources ([www.agilent.com](http://www.agilent.com)).

Experienced Agilent test engineers throughout the world offer practical recommendations for product evaluation and selection. After you purchase an Agilent product, they can provide no-charge assistance with operation verification and basic measurement setups for advertised capabilities. To enhance the features, performance, and flexibility of your test and measurement products—and to help you solve application challenges—Agilent offers free or extra-cost product options and upgrades, and sell expert engineering, calibration, and other consulting services.

### Phone and fax

United States:  
Agilent Technologies  
(tel) 1 800 452 4844

Canada:  
Agilent Technologies Canada Inc.  
(tel) 1 877 894 4414

Europe:  
Agilent Technologies  
Test & Measurement  
European Marketing Organisation  
(tel) (31 20) 547 2000

Japan:  
Agilent Technologies Japan Ltd.  
(tel) (81) 426 56 7832  
(fax) (81) 426 56 7840

Latin America:  
Agilent Technologies  
Latin American Region Headquarters, U.S.A.  
(tel) (305) 267 4245  
(fax) (305) 267 4286

Australia/New Zealand:  
Agilent Technologies Australia Pty Ltd.  
(tel) 1 800 629 485 (Australia)  
(fax) (61 3) 9272 0749  
(tel) 0 800 738 378 (New Zealand)  
(fax) (64 4) 802 6881

Asia Pacific:  
Agilent Technologies, Hong Kong  
(tel) (852) 3197-7777  
(fax) (852) 2506-9284

Data Subject to Change  
© Agilent Technologies 2000  
Printed in the U.S.A. 04/2000  
Publication No.: 5966-2384E



**Agilent Technologies**  
Innovating the HP Way