
HP E7347A and HP E7357A Performance Upgrade Kits for HP Network Analyzers

Installation Manual

Applicable systems:

HP 85106C with Options 001 and 002
HP 85106D with Option 001
HP 85109C with Option 002

HP part number: E7350-90005
Printed in USA
June 1998

Revision 1.0

Notice

The information contained in this document is subject to change without notice.

Hewlett-Packard makes no warranty of any kind with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Hewlett-Packard shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Hewlett-Packard assumes no responsibility for the use or reliability of its software on equipment that is not furnished by Hewlett-Packard.

This document contains proprietary information which is protected by copyright. All rights are reserved. No part of this document may be photocopied, reproduced, or translated to another language without prior written consent of Hewlett-Packard Company.

Restricted Rights Legend

Use, duplication, or disclosure by the U.S. Government is subject to restrictions as set forth in subparagraph (c)(1)(ii) of the Rights in Technical Data and Computer Software clause at DFARS 252.227-7013 for DOD agencies, and subparagraphs (c)(1) and (c)(2) of the Commercial Computer Software Restricted Rights clause at FAR 52.227-19 for other agencies.

Hewlett-Packard Company
Santa Rosa Systems Division
1400 Fountaingrove Parkway
Santa Rosa, CA 95403-1799, U.S.A.

© Copyright Hewlett-Packard Company 1998

Read Me First!

Using this document and an HP E7347A or HP E7357A upgrade package, an HP service engineer can upgrade select HP network analyzers to full HP 8510XF capability, in either 85 GHz or 110 GHz.

NOTE

Hewlett-Packard does not recommend customer installation of the upgrade packages.

Network Analyzer Upgrade Options

HP 85106C, Option 001 and Option 002

- added the HP 8517B,
- replaced the HP 83621A/B with the HP 83651A/B, and
- replaced the HP 8350B/83540A with the HP 83621A/B.

HP 85106D, Option 001

- added the HP 8517B, and
- replaced the HP 83621B with the HP 83651B.

HP 85109C, Option 002

- replaced the HP 8350B/83540A with the HP 83621A/B.

Scheduling Installation

The HP E7347A or HP E7357A performance upgrade packages come with prepaid installation. Please call your local Hewlett-Packard sales and service office to arrange for a service engineer to install the upgrade kit. Call toll free, 1-800-593-6635, or refer to “Service and Support”.

Warranty

Certification

Hewlett-Packard Company certifies that this product met its published specifications at the time of shipment from the factory. Hewlett-Packard further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology (NIST, formerly NBS), to the extent allowed by the Institute's calibration facility, and to the calibration facilities of other International Standards Organization members.

NOTE

If a Hewlett-Packard service engineer installs the E7347A or HP E7357A upgrade package, the upgraded millimeter-wave subsystem and the additional source have an on-site warranty of 1 year following the installation date. The remainder of the HP 85107B system warranty does not change.

Warranty

This Hewlett-Packard system product is warranted against defects in materials and workmanship for a period corresponding to the individual warranty periods of its component products. Instruments are warranted for a period of one year. During the warranty period, Hewlett-Packard Company will, at its option, either repair or replace products that prove to be defective.

Warranty service for products installed by HP and certain other products designated by HP will be performed at Buyer's facility at no charge within HP service travel areas. Outside HP service travel areas, warranty service will be performed at Buyer's facility only upon HP's prior agreement and Buyer shall pay HP's round trip travel expenses. In all other areas, products must be returned to a service facility designated by HP.

For products returned to HP for warranty service, Buyer shall prepay shipping charges to HP and HP shall pay shipping charges to return the product to Buyer. However, Buyer shall pay all shipping charges, duties, and taxes for products returned to HP from another country.

HP warrants that its software and firmware designated by HP for use with an instrument will execute its programming instructions when properly installed on that instrument. HP does not warrant that the operation of the instrument, or software, or firmware will be uninterrupted or error free.

LIMITATION OF WARRANTY. The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by Buyer, Buyer-supplied software or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

NO OTHER WARRANTY IS EXPRESSED OR IMPLIED. HP SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OR MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

EXCLUSIVE REMEDIES. THE REMEDIES PROVIDED HEREIN ARE BUYER'S SOLE AND EXCLUSIVE REMEDIES. HP SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER BASED ON CONTRACT, TORT, OR ANY OTHER LEGAL THEORY.

Assistance

Product maintenance agreements and other customer assistance agreements are available for Hewlett-Packard products.

For assistance, call your local Hewlett-Packard Sales and Service Office (refer to "Service and Support" on page vi).

Service and Support

Any adjustment, maintenance, or repair of this product must be performed by qualified personnel. Contact your customer engineer through your local HP Service Center. You can find a list of HP Service Centers on the web at <http://www.hp.com/go/tmdir>.

If you do not have access to the Internet, one of these HP centers can direct you to your nearest HP representative:

United States:	Hewlett-Packard Company Test and Measurement Call Center PO Box 4026 Englewood, CO 80155-4026 (800) 452 4844 (toll-free in US)
Canada:	Hewlett-Packard Canada Ltd. 5150 Spectrum Way Mississauga, Ontario L4W 5G1 (905) 206 4725
Europe:	Hewlett-Packard European Marketing Centre Postbox 999 1180 AZ Amstelveen The Netherlands (31 20) 547 9900
Japan:	Yokogawa-Hewlett-Packard Ltd. Measurement Assistance Center 9-1, Takakura-Cho, Hachioji-Shi Tokyo 192, Japan (81) 426 56 7832 (81) 426 56 7840 (FAX)
Latin America:	Hewlett-Packard Latin American Region Headquarters 5200 Blue Lagoon Drive, 9th Floor Miami, Florida 33126, U.S.A. (305) 267 4245 (305) 267 4288 (FAX)
Australia/New Zealand:	Hewlett-Packard Australia Ltd. 31-41 Joseph Street Blackburn, Victoria 3130 Australia 1 800 629 485 (toll-free)
Asia-Pacific:	Hewlett-Packard Asia Pacific Ltd. 17-21/F Shell Tower, Times Square 1 Matheson Street, Causeway Bay Hong Kong (852) 2599 7777 (852) 2506 9285 (FAX)

Safety and Regulatory Information

Review this product and related documentation to familiarize yourself with safety markings and instructions before you operate the instrument. This product has been designed and tested in accordance with international standards.

WARNING

The WARNING notice denotes a hazard. It calls attention to a procedure, practice, or the like, that, if not correctly performed or adhered to, could result in personal injury. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

CAUTION

The **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like, which, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

Instrument Markings



When you see this symbol on your instrument, you should refer to the instrument's instruction manual for important information.



This symbol indicates hazardous voltages.



The laser radiation symbol is marked on products that have a laser output.



This symbol indicates that the instrument requires alternating current (ac) input.



The CE mark is a registered trademark of the European Community. If it is accompanied by a year, it indicates the year the design was proven.



The CSA mark is a registered trademark of the Canadian Standards Association.

1SM1-A This text indicates that the instrument is an Industrial Scientific and Medical Group 1 Class A product (CISPER 11, Clause 4).



This symbol indicates that the power line switch is ON.



This symbol indicates that the power line switch is OFF or in STANDBY position.

Safety Earth Ground



This is a Safety Class I product (provided with a protective earthing terminal). An uninterruptible safety earth ground must be provided from the main power source to the product input wiring terminals, power cord, or supplied power cord set. Whenever it is likely that the protection has been impaired, the product must be made inoperative and secured against any unintended operation.

Before Applying Power

Verify that the product is configured to match the available main power source as described in the input power configuration instructions in this manual. If this product is to be powered by autotransformer, make sure the common terminal is connected to the neutral (grounded) side of the ac power supply.

Typeface Conventions

- | | |
|---------------------------|---|
| <i>Italics</i> | <ul style="list-style-type: none">• Used to emphasize important information:
Use this software <i>only</i> with the HP xxxxxX system.• Used for the title of a publication:
Refer to the <i>HP xxxxxX System-Level User's Guide</i>.• Used to indicate a variable:
Type <code>LOAD BIN filename</code>. |
| Instrument Display | <ul style="list-style-type: none">• Used to show on-screen prompts and messages that you will see on the display of an instrument:
The HP xxxxxX will display the message <code>CAL1 SAVED</code>. |
| [Keycap] | <ul style="list-style-type: none">• Used for labeled keys on the front panel of an instrument or on a computer keyboard:
Press [Return]. |
| {Softkey} | <ul style="list-style-type: none">• Used for simulated keys that appear on an instrument display:
Press {Prior Menu}. |
| User Entry | <ul style="list-style-type: none">• Used to indicate text that you will enter using the computer keyboard; text shown in this typeface must be typed <i>exactly</i> as printed:
Type <code>LOAD PARMFILE</code>• Used for examples of programming code:
<code>#endif // ifndef NO_CLASS</code> |
| <i>Path Name</i> | <ul style="list-style-type: none">• Used for a subdirectory name or file path:
Edit the file <code>usr/local/bin/sample.txt</code> |
| Computer Display | <ul style="list-style-type: none">• Used to show messages, prompts, and window labels that appear on a computer monitor:
The Edit Parameters window will appear on the screen.• Used for menus, lists, dialog boxes, and button boxes on a computer monitor from which you make selections using the mouse or keyboard:
Double-click EXIT to quit the program. |

Introduction

Contents:

- “Scheduling Installation” on page -2
- “System Configurations” on page -3
- “Overview of the Upgrade Packages” on page -5
- “Installation Procedure Outline” on page -6
- “Step 1. Secure Static Safe Work Station” on page -8
- “Step 2. Verify Upgrade Package Contents” on page -9
- “Step 3. Secure Additional Installation Equipment” on page -11
- “Step 4. Check the Network Analyzer System Operation and Memory” on page -12
- “Step 5. Install Non-Volatile Memory Upgrade (if needed)” on page -13
- “Step 6. Disconnect Unneeded Equipment” on page -16
- “Step 7. Install the Millimeter Wave Controller” on page -17
- “Step 8. Install the Millimeter Wave Test Set” on page -18
- “Step 9. Reconnect the System” on page -19
- “Step 10. Load HP 8510XF Operating System (Firmware)” on page -21
- “Step 11. Perform the HP 8510XF Performance Verification” on page -22

NOTE

The HP 8510C works with all HP 8360 synthesized sweeper models. To take advantage of two HP 8510C system features (quick step and test port power flatness correction), however, some HP 8360 instruments must be upgraded.

Scheduling Installation

The HP E7347A and E7357A performance upgrade packages come with prepaid installation. Please call your local Hewlett-Packard sales and service office to arrange for a service engineer to install the upgrade kit. Call toll free, 1-800-593-6635, or refer to “Service and Support” in the front of this manual.

NOTE

Hewlett-Packard does not recommend customer installation of these upgrade packages. Customer installation of these upgrade packages will void the warranty.

System Configurations

The system may be configured either for coaxial measurement or on-wafer measurement.

Coaxial Configuration

When the HP 8510XF is configured for measurement through coaxial connections, the network analyzer, millimeter wave controller, and RF and LO sources are all installed in the system rack as shown in Figure 1. The test heads are placed on a work surface which is mounted below the millimeter wave controller.

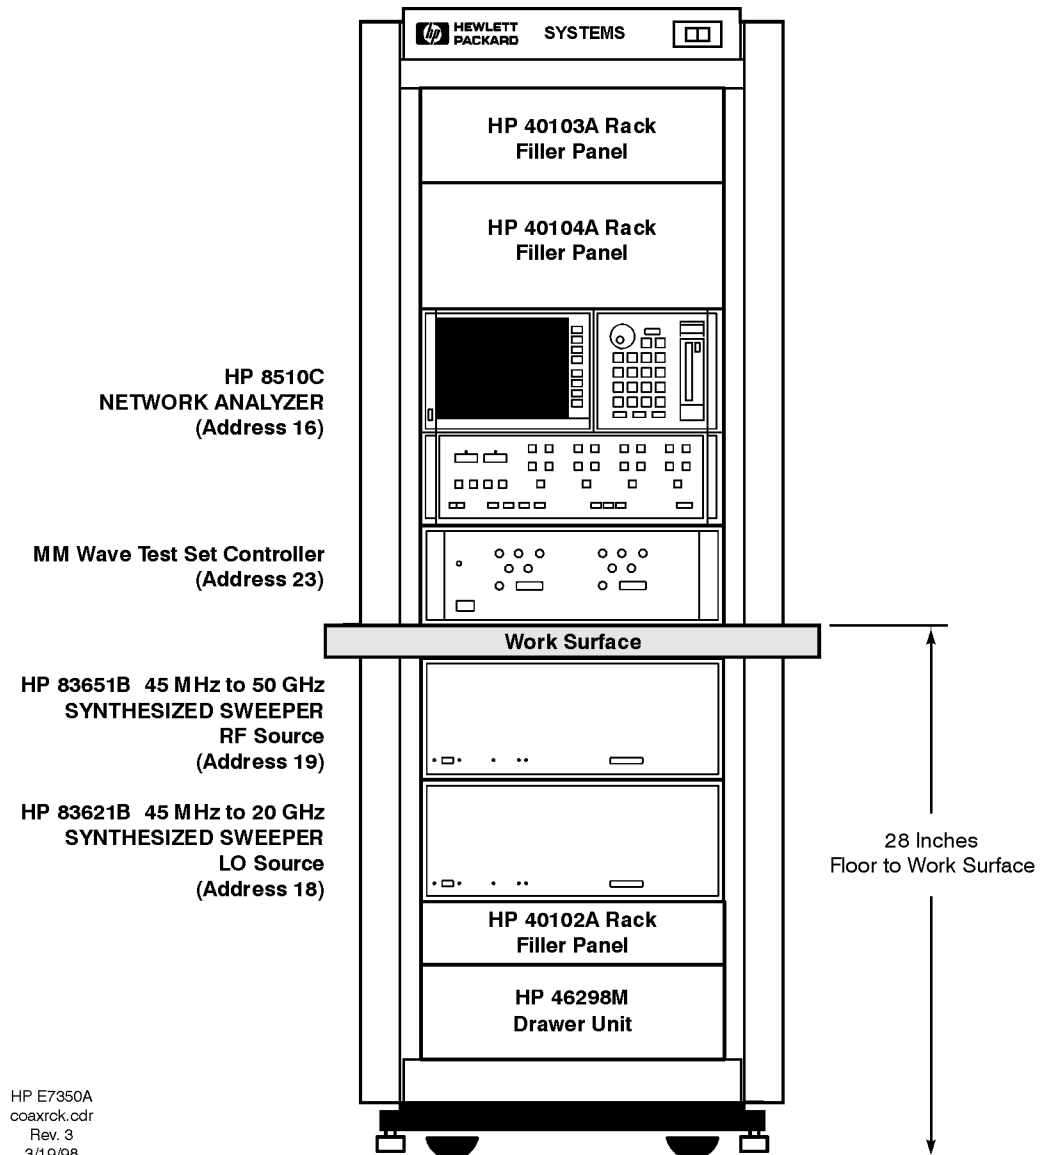


Figure 1 Network analyzer mounted in system rack

**Wafer Probe
Configuration**

When the HP 8510XF is configured for measurement through on-wafer probe connections, the millimeter wave controller, and the RF and LO sources are installed in the rack. However, the network analyzer and the wafer probe station are placed side-by-side on a work surface in front of the test system, as shown in Figure 2.

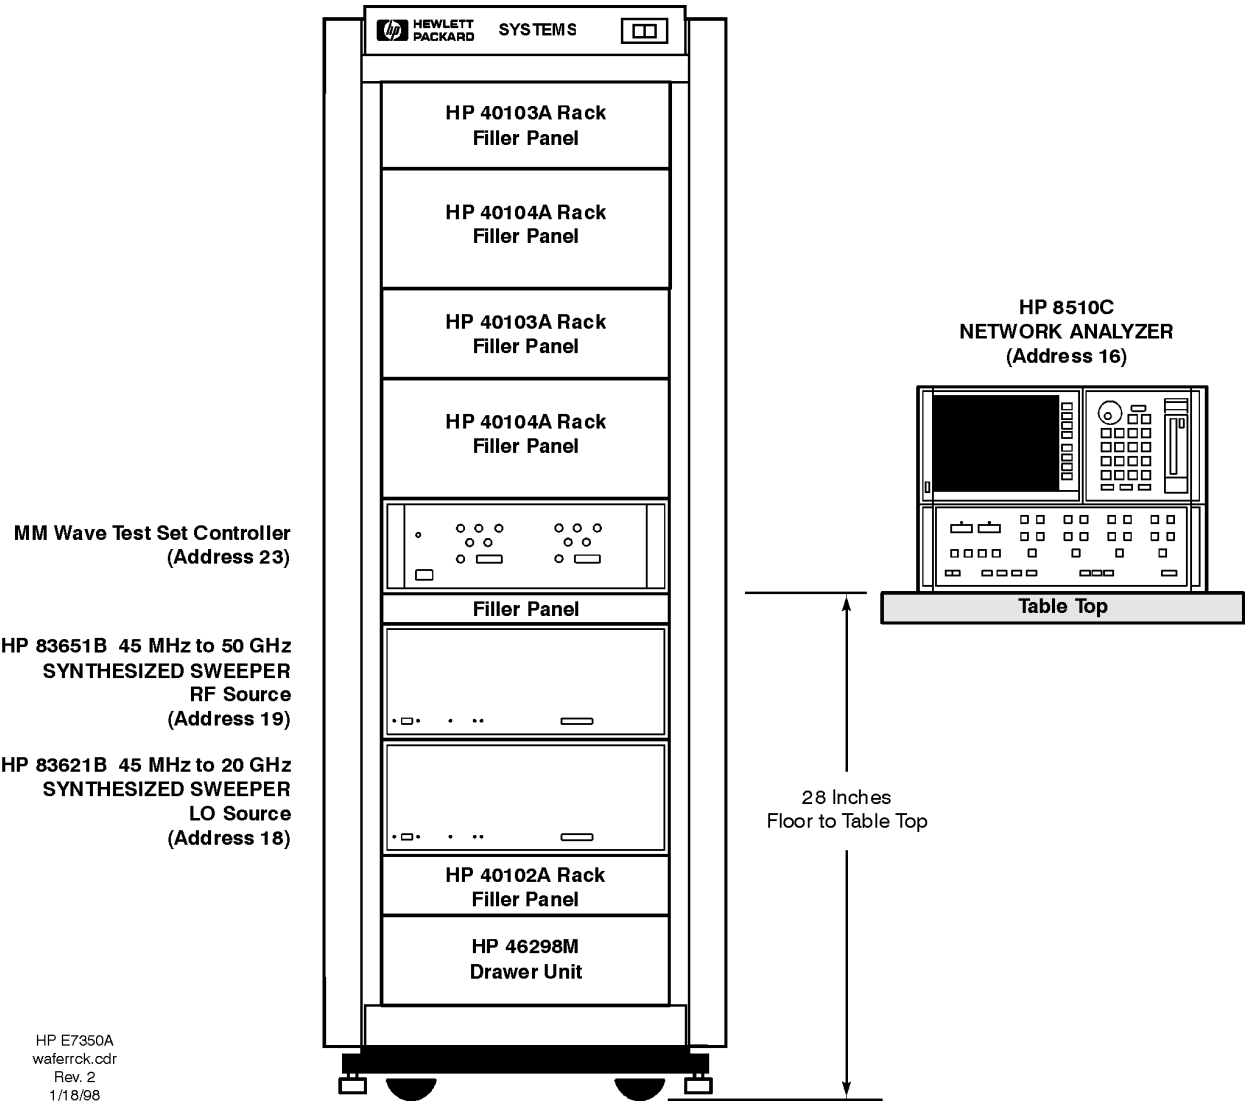


Figure 2 Network analyzer located on work surface

Overview of the Upgrade Packages

The HP E7347A or HP E7357A upgrade packages will upgrade a designated existing network analyzer system to the HP 8510XF system with 85 GHz or 110 GHz capability, respectively.

HP 8510XF (85 GHz)

Use the HP E7347A package to upgrade a designated network analyzer to an HP 8510XF with 85 GHz capability. With this package, you will do the following:

- Check the operation of the network analyzer.
- Check the memory in HP 8510C vector network analyzer.
- Upgrade the memory in the HP 8510C vector network analyzer.
- Disconnect unwanted elements from the existing system.
- Install an HP E7341A millimeter wave controller.
- Install millimeter wave test set.
- Reconnect the system.
- Load the HP 8510XF operating system.
- Use the HP 8510C performance verification software to verify performance of HP 8510XF in coax.

HP 8510XF (110 GHz)

Use the HP E7357A package to upgrade a designated network analyzer to an HP 8510XF with 110 GHz capability. With this package, you will do the following:

- Check the operation of the network analyzer.
- Check the memory in HP 8510C vector network analyzer.
- Upgrade the memory in the HP 8510C vector network analyzer.
- Disconnect unwanted elements from the existing system.
- Install an HP E7341A millimeter wave controller.
- Install millimeter wave test set.
- Reconnect the system.
- Load the HP 8510XF operating system.
- Use the HP 8510C performance verification software to verify performance of HP 8510XF in coax.

Installation Procedure Outline

Follow this outline to install either the HP E7347A or E7357A performance upgrade. Detailed procedures are provided in the subsequent sections.

Step 1 Secure a Static Safe Work Station

Check for the following:

- the static mat sits on a clean, flat, sturdy surface.
- the static mat has a connection to an earth ground.
- the static mat has a wrist strap connected to it.

Step 2 Verify the Upgrade Package Contents

Using the packing list for your upgrade kit, check the completeness of the package. If the kit does not have all the items listed, contact your local Hewlett-Packard office (see table inside the front of this manual).

Step 3 Secure Items Not Included in Upgrade Package

Using the table provided in this section, obtain the items required but not supplied in the package.

Step 4 Check the Existing Network Analyzer System Operation and Memory

Using the instructions in this section, check that the system you plan to upgrade functions.

Step 5 Install Non-Volatile Memory Upgrade (if needed)

Using the instructions in this section, install additional memory in the HP 8510C.

Step 6 Disconnect Unneeded Equipment

Using the instructions in this section, disconnect the equipment not needed for the upgraded system and remove them from the system rack.

Step 7 Install the Millimeter Wave Controller

Using the instructions in this section, install the HP E7341A millimeter wave controller.

Step 8 Reconnect the System

Using the instructions in this section, reconnect the system.

Step 9 Install the Millimeter Wave Test Set

Using the instructions in this section, install the millimeter wave test set.

Step 10 Load the HP 8510XF Operating System (Firmware)

Using the instructions in this section, load the HP 8510XF operating system.

Step 11 Performance Check the Upgraded HP 8510XF System

Using the instructions in this section, performance check the upgraded network analyzer system.

Step 1. Secure Static Safe Work Station

Static electricity builds up on the body and on tools, including calibration components and devices under test. When static electricity is accidentally discharged, sensitive circuit elements can be damaged.

CAUTION

It is important that appropriate measures are taken to adequately discharge static electricity which may otherwise damage test equipment circuitry.

Circuit elements within a device can be damaged from static electricity, such as through accidental contact with the center conductor of a connector. Even a discharge that is too small to be felt can cause circuit damage.

Protection against electrostatic discharge (ESD) is essential while connecting, cleaning, or inspecting connectors attached to static-sensitive circuits, such as those found in test sets. Protective measures appropriate to the HP 8510 series systems are described below.

- Always use a grounded anti-static mat in front of your test equipment, and wear a grounded wrist strap attached to it.
- Ground yourself before you clean, inspect, or make a connection to a static-sensitive device or test port. You can, for example, grasp the grounded outer shell of the test port briefly to discharge static from your body.
- Discharge static electricity from a device before connecting it, such as by touching the device briefly through a resistor of at least 1 M Ω to either the outer shell of the test port or to another exposed ground.

ESD Accessories

The following accessories for preventing electrostatic discharge can be ordered from Hewlett-Packard:

Item	HP Part Number
Grounding wrist strap	9300-1367
Grounding cord for wrist strap (5 ft)	9300-0980
Conductive table mat (2 x 4 ft) with ground wire (15 ft)	9300-0797
ESD heel strap (for conductive floors)	9300-1126

Step 2. Verify Upgrade Package Contents

Following are the contents of the HP E7347A and E7357A performance upgrade packages. Compare this list against the packing list and against the actual package contents. If the kit does not have all of the items listed, contact your nearest Hewlett-Packard office.

Table 1 *Performance Upgrade Package Contents*

Item	HP Part Number	HP E7347A Quantity	HP E7357A Quantity
Software Data Disk	08510-10033	1	1
Cable, IF Interconnect	08510-60107	1	1
Cable, IF Interconnect	08510-60126	2	2
Adapter, 2.4mm (f-f)	11900B	1	1
IC EEPROM, 32K X 8 (Memory Chips)	1818-7167	8	8
Adapter, 3.5mm (f-f)	5061-5311	1	1
Power Cable, 03C 03f-03m	8120-1348	2	2
Power Cable, 03C 03F-03M	8120-1405	1	1
Power Cable, 03C 03F-03M (Opt. 230)	8120-1575	1	1
Power Cable, 03C 03f-03m (for Opt. 230)	8120-1763	2	2
Cable Assembly, BNC	8120-1838	1	1
Cable Assembly, BNC	8120-1839	1	1
Cable, HP-IB	8120-3447	1	1
Cable Assembly, BNC	8120-5370	2	2
HP 8510XF Operating System	E7340-10001	1	1
Semirigid Cable	E7340-20075	1	1
Semirigid Cable	E7340-20076	1	1
Cable, DC Bias	E7340-60009	2	2
Millimeter Controller	E7341A	1	1
Head Assembly, Left	E7342L	1	0
Head Assembly, Right	E7342R	1	0
RF Cable, SMA-SMA (Opt. 005)	E7342-60003	4	4
LO Cable, 3.5mm-3.5mm	E7342-60004	2	2
RF Cable, 2.4mm	E7342-60005	4	4

Table 1 Performance Upgrade Package Contents (Continued)

Item	HP Part Number	HP E7347A Quantity	HP E7357A Quantity
Head Assembly, Left	E7352L	0	1
Head Assembly, Right	E7352R	0	1
System Manual	E7350-90001	1	1
Upgrade Installation Manual	E7350-90005	1	1

Step 3. Secure Additional Installation Equipment

Equipment Required But Not Supplied

The following additional equipment will aid in the installation of the upgrade package, but are *not* included in the upgrade kit.

Make sure that these items are available and at hand before proceeding with the upgrade.

Table 2 *Equipment Required But Not Supplied*

Item	HP Part Number
Network Analyzer	8510C
Sources	83650B or 83651B, and 83620B or 83621B
Test Set (optional)	8517B
Calibration/Verification kit	85059A
HP-IB cables	10388A
BNC to BNC cable	10503A
Small Pozi-drive (#1)	8710-0899
Medium Pozi-drive (#2)	8710-0900
Flat blade screwdriver	8730-0001
Static control table mat	9300-0797
Wrist strap	9300-1367
Wrist-strap-to-mat cord (5 ft)	9300-1980
PC with HP BASIC for Windows (Rev. 6.3 or higher)	N/A

Step 4. Check the Network Analyzer System Operation and Memory

The following information applies to both the HP E7347A and E7357A upgrade kits. Use this procedure to ensure that the existing network analyzer system works properly before installing the upgrade package.

Procedure

1. Turn on the instruments in the following order:
 - a. the HP 83651B and 83621B sources (be sure to turn the switch to power on, not standby)
 - b. the HP 85105 test set controller
 - c. the HP 8510C network analyzer
2. On the HP 85102, press the green preset key.
3. Does the system pass self-test (HP 85101 self tests, 85102 running error messages, and test set unratio of power tests) and display a **LOG MAG S₁₁** trace? If not, do *not* perform the upgrade until the system has been serviced.
4. Initialize a blank disk, as follows:
 - a. load a blank diskette (with write-protect off),
 - b. on the HP 85102, press **DISK**,
 - c. on the HP 85101, select **INITIALIZE DISK: YES**.
5. Does the system initialize the disk and display **DISK INITIALIZED**? If not, tag the HP 85101, indicating that it has a defective disk drive. The disk drive must be working to load the HP 8510XF firmware.
6. Turn the CRT to its highest intensity. Does the image remain focused? If not, return the CRT to its normal intensity and tag the HP 85101, indicating that it has a defective CRT.
7. Return the CRT to its normal intensity. As long as the CRT functions properly, continue with this procedure.
8. If the system displays a self-test,* running error message, or unratioed power test failure, check the equipment setup. Do not perform the upgrade until either you correct the setup problem, or you have the system serviced.

* You may have to rely on the red LEDs rather than the CRT.

Step 5. Install Non-Volatile Memory Upgrade (if needed)

The HP 8510XF firmware requires at least 832 Kbytes of non-volatile memory.

To determine how much memory is installed in the system

1. With the network analyzer system on, press [SYSTEM] {More} {Service Functions} {Test Menu}.
2. Select 22: run service program.
3. Select 1: 85101 Display/processor service program.
4. Select 4: non-volatile memory board.
5. A password is required, which is "8515".

CAUTION

Incorrect usage of the password can erase the non-volatile memory.

6. Select 8. If the *Number of Pages* reading is equal to or greater than 30BB, there is enough memory for running the HP 8510XF firmware. Skip the balance of this procedure and go to "Step 6. Disconnect Unneeded Equipment" on page -16.

To increase the non-volatile memory

1. Place the HP 8510C on an ESD safe work surface and insure there is no AC power connected to the rear panel.
2. Remove the two plastic feet on the rear upper portion of the HP 8510C, and then remove the top cover. The PC boards are located beneath the metal cover that runs the length of the right side of the chassis.
3. Remove the 21 screws that secure the cover and remove the cover to access the PC boards. The board that contains the non-volatile memory is the A6 board, and is easily identified by its orange card extractor.
4. Remove the plastic card spacers that position the A6 board.
5. Gently grab the card extractor tabs on the ends of the board, and pull away and up to remove the board.
6. Place the board on an ESD safe work surface. There are 16 banks on the board, and HP 8510XF requires at least 13 banks. There are 8 IC chips supplied with this kit. Fill the empty slots until at least 13 banks are filled. The ICs to be loaded in these sockets are a CMOS version of the original replacement IC (HP part number 1818-4653).

7. Carefully bend the leads of the IC chips so that the leads are perpendicular to the body and insert them into the empty sockets. Be sure to match up the notch on the top of the chips with the notch on the sockets. Gently press them into place making sure that all leads go into the socket.
8. After the ICs have been installed, gently insert the A6 board back into its connector.

Verify the memory upgrade with chassis open

9. Plug the power cord into the HP 85101C, turn on the power, and allow the instrument to complete its initialization.
10. With the HP 85101C box on, press [=marker] to enter the **Test** menu.
11. Select **22: run service program**.
12. Select **1: 85101 Display/processor service program**.
13. Select **4: non-volatile memory board**.
14. A password is required, which is "8515".

CAUTION

Incorrect useage of the password can erase the non-volatile memory.

15. Select **1:Initialize Memory**.
16. On the front panel of the HP 8510C, select **Prior Menu**, then **Show Non-Volatile Memory Parameters**. The HP 8510C should be displaying the memory board parameters. If the EEPROM in the highest memory page was read successfully, then the # of pages should read at least **30BB**. Ignore the present position information. The number-of-pages information is only useful for indicating whether the last bank of upgraded memory is good or not.

Memory Write/Read Test

17. To determine if all of the added memory banks are functioning, select **Prior Menu**, then **Complete Memory Board Unformatted Write/Read Test (2)**.
18. Press [=Marker] [x1]. This test takes a few minutes to run. If all the memory banks are working, the display will read that the first useable memory bank location is **10 hex**. If any other hex location is listed, refer to the following chart to determine which EEPROM chip is at fault.

First Unuseable Memory Location Read	Possible Fault Location
0C Hex	U13 or U29
0D Hex	U14 or U30
0E Hex	U15 or U31
0F Hex	U16 or U32

Try replacing one or the other or both of the EEPROMs listed if you do not get 10 Hex as the first useable memory location. Continue repeating the above test until the bad EEPROM(s) are identified.

19. When the EEPROMs are found to be working properly, turn off the HP 8510C and remove the power cord from the rear panel.
20. Reinstall the plastic spacers on the A6 board.
21. Place the cover over the PC board cage and secure the original 21 screws.
22. Install the top cover on the HP 8510C and finish integrating the HP 8510C into the system depending on the configuration.

Step 6. Disconnect Unneeded Equipment

If upgrading to an HP 8510XF with Option 006, the HP 8517B test set must have Option 001, multi-test set compatibility. If HP 8517B does not have Option 001 installed, you will need to order and install this upgrade kit (p/n 8511A K01).

If this is the case, the HP 8517B will need to be relocated to facilitate the millimeter wave controller. The HP 8517B should be removed from the rack and placed on the work surface or another rack. The HP 8517B should be placed as close to the millimeter wave controller as possible.

If the HP 8510XF does not include Option 006, then remove the HP 8517B from the test system prior to installing the upgrade.

Step 7. Install the Millimeter Wave Controller

Install the HP 7341A millimeter wave controller into the system rack as shown in Figure 1 (in-rack configuration) or Figure 2 (table-top configuration).

Adjust the position of the sources if needed.

Step 8. Install the Millimeter Wave Test Set

Using the following procedure, install the millimeter wave test set:

1. Place the test heads on the table top or work surface in front of the millimeter wave controller.
2. Connect the cables as shown in Figure 3. Installation of these cables may require a long, 5/16-inch open-ended wrench.

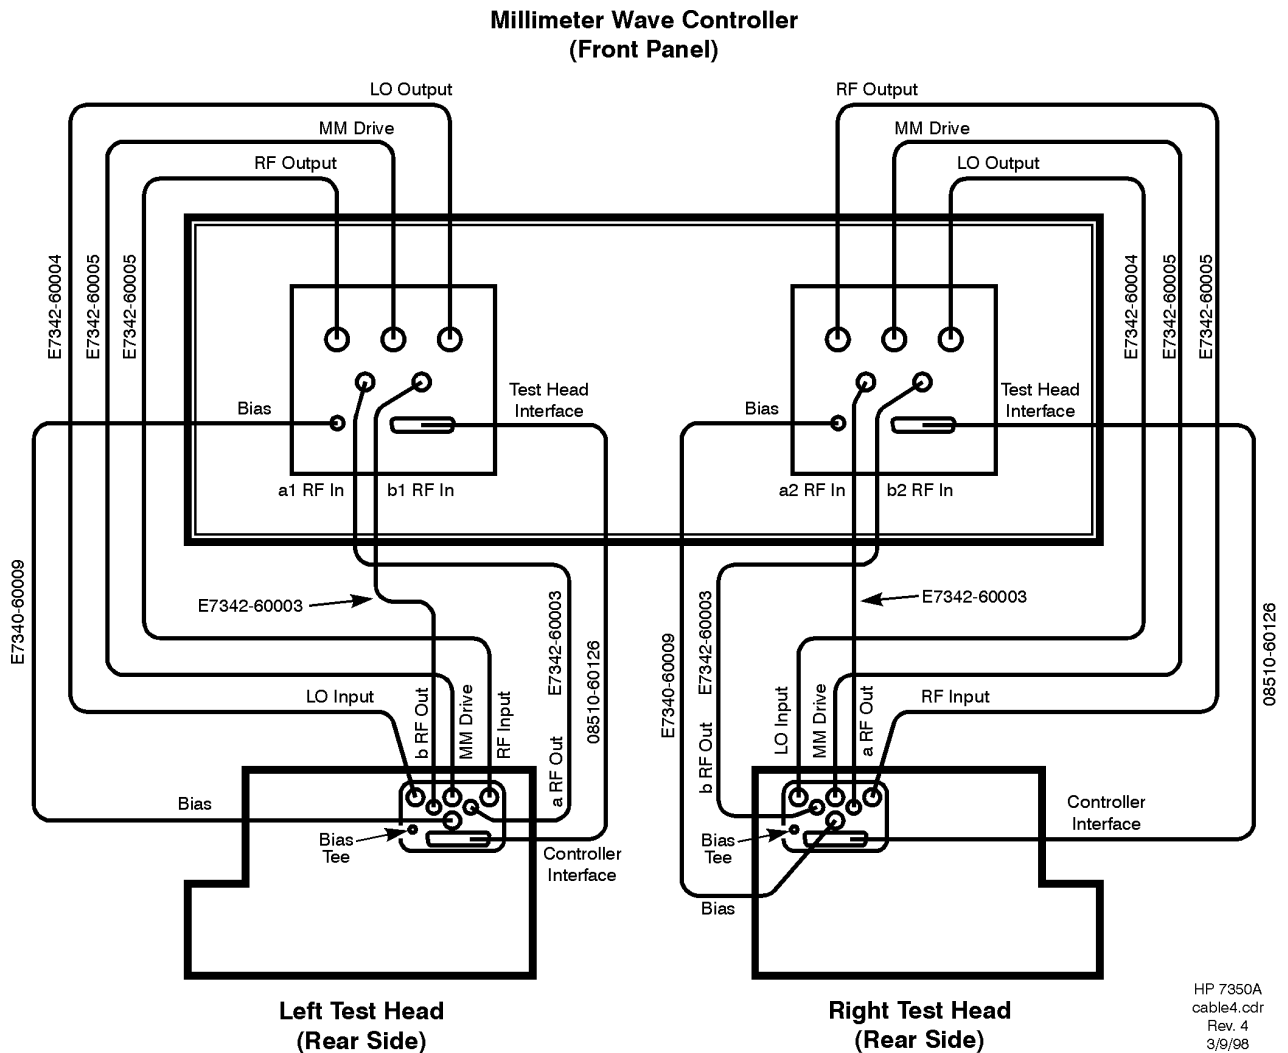


Figure 3 Controller to Test Heads Cabling

Step 9. Reconnect the System

Reconnect the test system according to the desired configuration. Figure 4 shows the system wiring for the coaxial configuration. Figure 5 shows the system wiring for the on-wafer configuration.

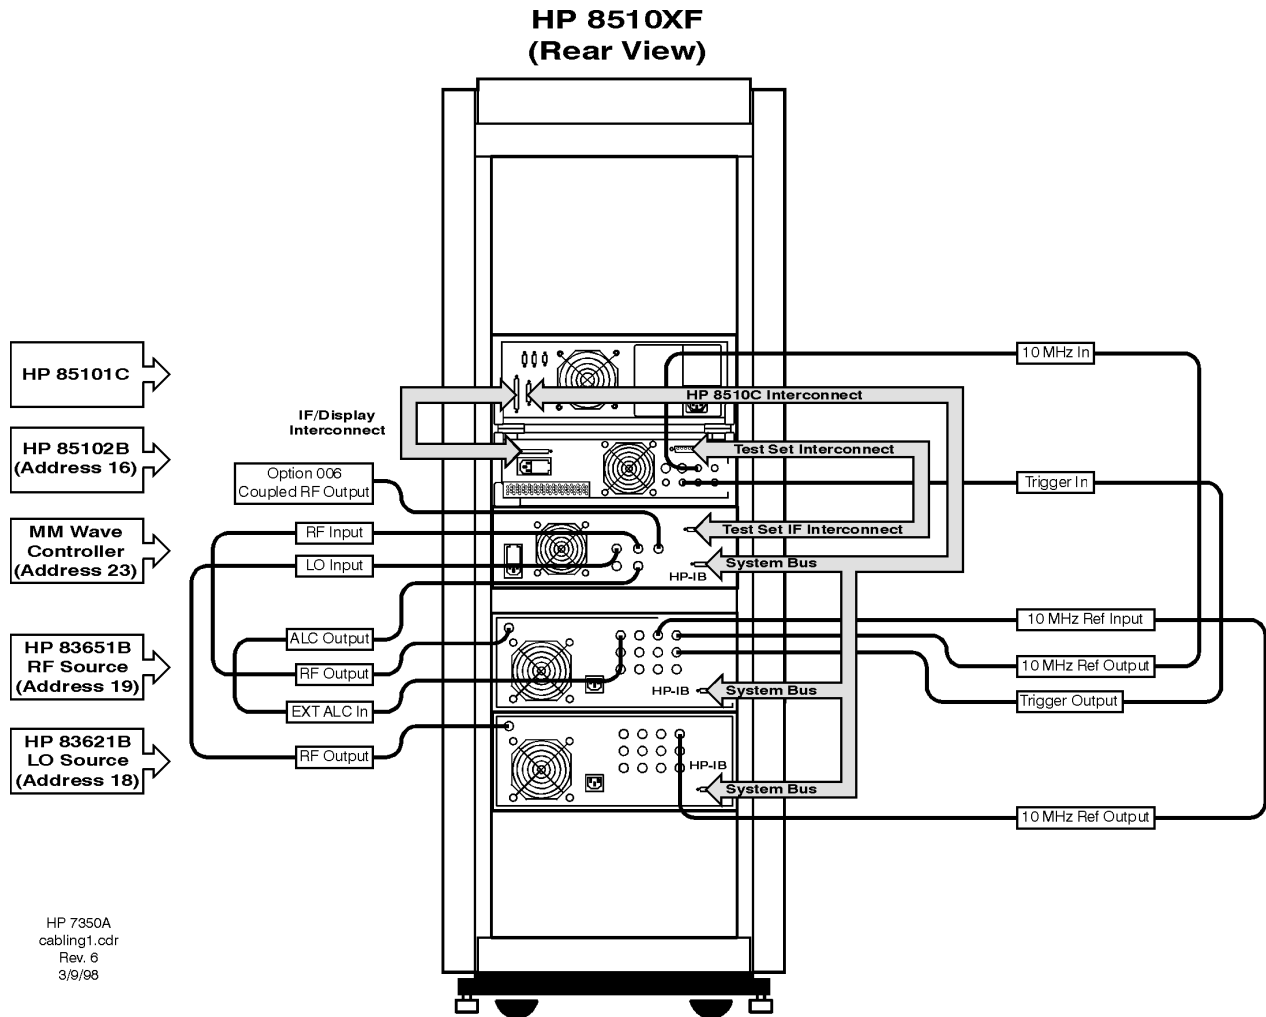


Figure 4 Coaxial configuration system cabling diagram

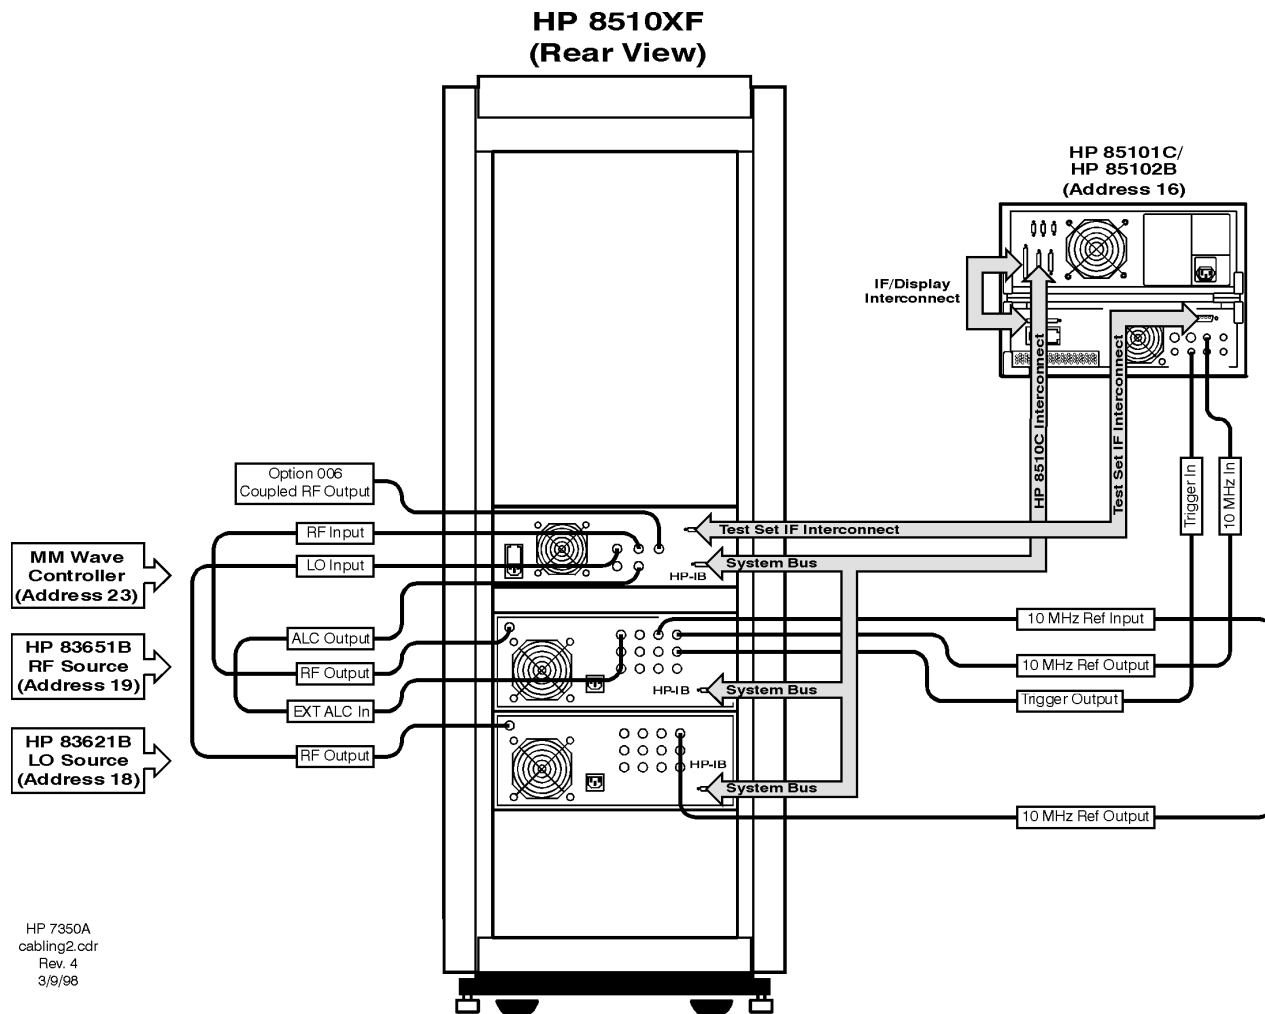


Figure 5 On-wafer configuration system cabling diagram

Step 10. Load HP 8510XF Operating System (Firmware)

Perform the following procedure to load the HP 8510XF software.

1. Insert the operating system disk into the HP 85101 disk drive.
2. On the HP 8510C, press [SYSTEM] *{More}*, and then select *{Service Function}*.
3. Select *{Test Menu}*, and then **19**. It takes about 3 minutes to load the software and reinitialize the system.

Step 11. Perform the HP 8510XF Performance Verification

Refer to the HP 8510XF System Manual for the procedures to perform a Performance Verification on the upgraded system.