# Model 7700, 7702, and 7703 Multiplexer Modules

## User's Guide

PA-695 Rev. D / October 2006



### WARRANTY

Keithley Instruments, Inc. warrants this product to be free from defects in material and workmanship for a period of 1 year from date of shipment.

Keithley Instruments, Inc. warrants the following items for 90 days from the date of shipment: probes, cables, rechargeable batteries, diskettes, and documentation.

During the warranty period, we will, at our option, either repair or replace any product that proves to be defective.

To exercise this warranty, write or call your local Keithley representative, or contact Keithley headquarters in Cleveland, Ohio. You will be given prompt assistance and return instructions. Send the product, transportation prepaid, to the indicated service facility. Repairs will be made and the product returned, transportation prepaid. Repaired or replaced products are warranted for the balance of the original warranty period, or at least 90 days.

### LIMITATION OF WARRANTY

This warranty does not apply to defects resulting from product modification without Keithley's express written consent, or misuse of any product or part. This warranty also does not apply to fuses, software, non-rechargeable batteries, damage from battery leakage, or problems arising from normal wear or failure to follow instructions.

THIS WARRANTY IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR USE. THE REMEDIES PROVIDED HEREIN ARE BUYER'S SOLE AND EXCLUSIVE REMEDIES.

NEITHER KEITHLEY INSTRUMENTS, INC. NOR ANY OF ITS EMPLOYEES SHALL BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING OUT OF THE USE OF ITS INSTRUMENTS AND SOFTWARE EVEN IF KEITHLEY INSTRUMENTS, INC., HAS BEEN ADVISED IN ADVANCE OF THE POSSIBILITY OF SUCH DAMAGES. SUCH EXCLUDED DAMAGES SHALL INCLUDE, BUT ARE NOT LIMITED TO: COSTS OF REMOVAL AND INSTALLATION, LOSSES SUSTAINED AS THE RESULT OF INJURY TO ANY PERSON, OR DAMAGE TO PROPERTY.



A GREATER MEASURE OF CONFIDENCE

Keithley Instruments, Inc.

Corporate Headquarters • 28775 Aurora Road • Cleveland, Ohio 44139 440-248-0400 • Fax: 440-248-6168 • 1-888-KEITHLEY (534-8453) • www.keithley.com



# **Safety Precautions**

The following safety precautions should be observed before using this product and any associated instrumentation. Although some instruments and accessories would normally be used with non-hazardous voltages, there are situations where hazardous conditions may be present.

This product is intended for use by qualified personnel who recognize shock hazards and are familiar with the safety precautions required to avoid possible injury. Read and follow all installation, operation, and maintenance information carefully before using the product. Refer to the manual for complete product specifications.

If the product is used in a manner not specified, the protection provided by the product may be impaired.

The types of product users are:

Responsible body is the individual or group responsible for the use and maintenance of equipment, for ensuring that the equipment is operated within its specifications and operating limits, and for ensuring that operators are adequately trained.

Operators use the product for its intended function. They must be trained in electrical safety procedures and proper use of the instrument. They must be protected from electric shock and contact with hazardous live circuits.

Maintenance personnel perform routine procedures on the product to keep it operating properly, for example, setting the line voltage or replacing consumable materials. Maintenance procedures are described in the manual. The procedures explicitly state if the operator may perform them. Otherwise, they should be performed only by service personnel.

Service personnel are trained to work on live circuits, and perform safe installations and repairs of products. Only properly trained service personnel may perform installation and service procedures.

Keithley products are designed for use with electrical signals that are rated Measurement Category I and Measurement Category II, as described in the International Electrotechnical Commission (IEC) Standard IEC 60664. Most measurement, control, and data I/O signals are Measurement Category I and must not be directly connected to mains voltage or to voltage sources with high transient over-voltages. Measurement Category II connections require protection for high transient over-voltages often associated with local AC mains connections. Assume all measurement, control, and data I/O connections are for connection to Category I sources unless otherwise marked or described in the Manual.

Exercise extreme caution when a shock hazard is present. Lethal voltage may be present on cable connector jacks or test fixtures. The American National Standards Institute (ANSI) states that a shock hazard exists when voltage levels greater than 30V RMS, 42.4V peak, or 60VDC are present. A good safety practice is to expect that hazardous voltage is present in any unknown circuit before measuring.

Operators of this product must be protected from electric shock at all times. The responsible body must ensure that operators are prevented access and/or insulated from every connection point. In some cases, connections must be exposed to potential human contact. Product operators in these circumstances must be trained to protect themselves from the risk of electric shock. If the circuit is capable of operating at or above 1000 volts, no conductive part of the circuit may be exposed.

Do not connect switching cards directly to unlimited power circuits. They are intended to be used with impedance limited sources. NEVER connect switching cards directly to AC mains. When connecting sources to switching cards, install protective devices to limit fault current and voltage to the card.

Before operating an instrument, make sure the line cord is connected to a properly grounded power receptacle. Inspect the connecting cables, test leads, and jumpers for possible wear, cracks, or breaks before each use.

When installing equipment where access to the main power cord is restricted, such as rack mounting, a separate main input power disconnect device must be provided, in close proximity to the equipment and within easy reach of the operator.

For maximum safety, do not touch the product, test cables, or any other instruments while power is applied to the circuit under test. ALWAYS remove power from the entire test system and discharge any capacitors before: connecting or disconnecting cables or jumpers, installing or removing switching cards, or making internal changes, such as installing or removing jumpers.

Do not touch any object that could provide a current path to the common side of the circuit under test or power line (earth) ground. Always make measurements with dry hands while standing on a dry, insulated surface capable of withstanding the voltage being measured.

The instrument and accessories must be used in accordance with its specifications and operating instructions or the safety of the equipment may be impaired.

Do not exceed the maximum signal levels of the instruments and accessories, as defined in the specifications and operating information, and as shown on the instrument or test fixture panels, or switching card.

When fuses are used in a product, replace with same type and rating for continued protection against fire hazard.

Chassis connections must only be used as shield connections for measuring circuits, NOT as safety earth ground connections.

If you are using a test fixture, keep the lid closed while power is applied to the device under test. Safe operation requires the use of a lid interlock.

If a  $\left(\frac{\bot}{-}\right)$  screw is present, connect it to safety earth ground using the wire recommended in the user documentation.

The 1 symbol on an instrument indicates that the user should refer to the operating instructions located in the manual.

The symbol on an instrument shows that it can source or measure 1000 volts or more, including the combined effect of normal and common mode voltages. Use standard safety precautions to avoid personal contact with these voltages.

The  $\overrightarrow{m}$  symbol indicates a connection terminal to the equipment frame.

The WARNING heading in a manual explains dangers that might result in personal injury or death. Always read the associated information very carefully before performing the indicated procedure.

The CAUTION heading in a manual explains hazards that could damage the instrument. Such damage may invalidate the warranty.

Instrumentation and accessories shall not be connected to humans.

Before performing any maintenance, disconnect the line cord and all test cables.

To maintain protection from electric shock and fire, replacement components in mains circuits, including the power transformer, test leads, and input jacks, must be purchased from Keithley Instruments. Standard fuses, with applicable national safety approvals, may be used if the rating and type are the same. Other components that are not safety related may be purchased from other suppliers as long as they are equivalent to the original component. (Note that selected parts should be purchased only through Keithley Instruments to maintain accuracy and functionality of the product.) If you are unsure about the applicability of a replacement component, call a Keithley Instruments office for information.

To clean an instrument, use a damp cloth or mild, water based cleaner. Clean the exterior of the instrument only. Do not apply cleaner directly to the instrument or allow liquids to enter or spill on the instrument. Products that consist of a circuit board with no case or chassis (e.g., data acquisition board for installation into a computer) should never require cleaning if handled according to instructions. If the board becomes contaminated and operation is affected, the board should be returned to the factory for proper cleaning/servicing.

## 7700 20-Channel Differential Multiplexer w/Automatic CJC

#### **GENERAL**

20 CHANNELS: 20 channels of 2-pole relay input. All channels configurable to 4-pole.

2 CHANNELS: 2 channels of current only input.

RELAY TYPE: Latching electromechanical.

ACTUATION TIME: <3ms.

#### **CAPABILITIES**

CHANNELS 1-20: Multiplex one of 20 2-pole or one of 10 4-pole signals into DMM.

CHANNELS 21-22: Multiplex one of 2 2-pole current signals into DMM.

#### **INPUTS**

#### MAXIMUM SIGNAL LEVEL:

Channels (1-20): 300V DC or 300V rms (425V peak) for AC waveforms, 1A switched, 60W, 125VA maximum.

Channels (21-22): 60V DC or 30V rms, 3A switched, 60W, 125VA maximum

CONTACT LIFE (typ): >105 operations at max signal level.

>108 operations cold switching.

CONTACT RESISTANCE:  $<1\Omega$  at end of contact life.

**CONTACT POTENTIAL:** <±500nV typical per contact, 1μV max.

<±500nV typical per contact pair, 1µV max.

OFFSET CURRENT: <100pA.

CONNECTOR TYPE: Screw terminal, #20 AWG wire size.

ISOLATION BETWEEN ANY TWO TERMINALS: >1010Ω, <100pE

ISOLATION BETWEEN ANY TERMINAL AND EARTH: >10° $\Omega$ , <200pF.

CROSS TALK (50 $\Omega$  Load):

 $\label{eq:winternal} $$ w/Internal DMM $$ w/o Internal DMM^* $$ 10MHz: $$ <-40dB $$ <-40dB$ 

25MHz: \*\* <-25dB

 $^{\ast}$  Channels 24 and 25 are open. Refer to ROUTe: MULTiple command in 27xx User's manual.

\*\* Not valid

#### INSERTION LOSS (50 $\Omega$ Source, 50 $\Omega$ Load):

w/Internal DMM w/o Internal DMM\*
1MHz 1MHz

<0.1dB 1MHz 1MHz <3db 2MHz 50MHz

 $^{\ast}$  Channels 24 and 25 are open. Refer to ROUTe: MULTiple command in 27xx User's manual.

COMMON MODE VOLTAGE: 300V or 300V rms (425V peak) for AC waveforms between any terminal and chassis.

T/C COLD JUNCTION: 1.0°C (18°–28°C Mainframe Temp)

1.5°C (0°-18°C & 28°-50°C Mainframe Temp).


#### ENVIRONMENTAL:

**OPERATING ENVIRONMENT:** Specified for 0°C to 50°C.

Specified to 80% R.H. at 35°C.

STORAGE ENVIRONMENT:  $-25^{\circ}\text{C}$  to  $65^{\circ}\text{C}$ .

WEIGHT: 0.45kg (1 lb).

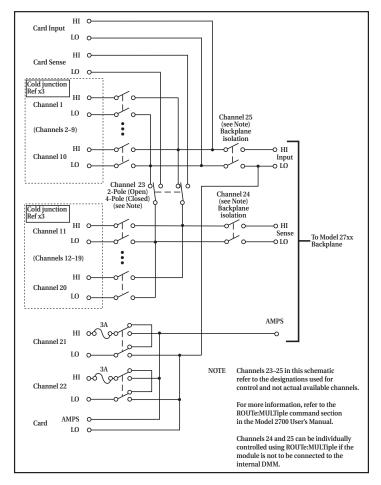

# 7702 40-Channel Differential Multiplexer

#### **GENERAL**

**40 CHANNELS:** 40 channels of 2-pole relay input. All channels configurable to 4-pole.

2 CHANNELS: 2 channels of current only input.

RELAY TYPE: Latching electromechanical.

ACTUATION TIME: <3ms.

#### **CAPABILITIES**

CHANNELS 1-40: Multiplex one of 40 2-pole or one of 20 4-pole signals into DMM.

CHANNELS 41-42: Multiplex one of 2 2-pole current signals into DMM.

#### **INPUTS**

#### **MAXIMUM SIGNAL LEVEL:**

Channels (1-40): 300V DC or rms, 1A switched, 60W, 125VA maximum.
Channels (41-42): 60V DC or 30V rms, 3A switched, 60W, 125VA maximum.

**CONTACT LIFE (typ):**  $>10^5$  operations at max signal level.

>108 operations cold switching.

**CONTACT RESISTANCE:**  $< 1\Omega$  at end of contact life.

CONTACT POTENTIAL: <±500nV typical per contact, 1µV max.

 $<\!\!\pm500 nV$  typical per contact pair,  $1\mu V$  max.

OFFSET CURRENT: <100pA.

CONNECTOR TYPE: Screw terminal, #20 AWG wire size.

ISOLATION BETWEEN ANY TWO TERMINALS:  $>10^{10}\Omega$ , <100pE

ISOLATION BETWEEN ANY TERMINAL AND EARTH: >109 $\Omega$ , <200pF.

CROSS TALK (10MHz,  $50\Omega$  Load): <-40dB.

 $\textbf{INSERTION LOSS (50} \Omega \textbf{ Source, 50} \Omega \textbf{ Load):} \qquad <0.1 dB \ below \ 1 MHz.$ 

<3dB below 2MHz.

COMMON MODE VOLTAGE: 300V between any terminal and chassis.


#### **ENVIRONMENTAL**

**OPERATING ENVIRONMENT:** Specified for 0°C to 50°C. Specified to 80% R.H. at 35°C.

STORAGE ENVIRONMENT: -25°C to 65°C.

WEIGHT: 0.5kg (1.1 lb).

Specifications subject to change without notice.

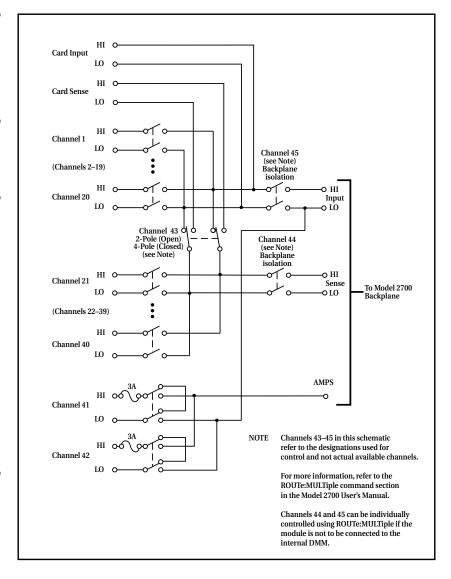

# 7703 32-Channel High Speed Differential Multiplexer

#### **GENERAL**

**32 CHANNELS:** 32 channels of 2-pole relay input. All channels configurable to 4-pole.

RELAY TYPE: Reed.

ACTUATION TIME: <1ms.

#### **CAPABILITIES**

CHANNELS 1-32: Multiplex one of 32 2-pole or one of 16 4-pole signals into DMM.

#### **INPUTS**

#### MAXIMUM SIGNAL LEVEL:

Channels (1-32): 300V DC or rms, 0.5A switched, 10W maximum.

Contact Life (typ):  $>5 \times 10^4$  operations at max signal level.  $>10^8$  operations cold switching.

**CONTACT RESISTANCE:**  $< 1\Omega$  at end of contact life.

CONTACT POTENTIAL: <±3µV typical per contact, 6µV max.

<±3μV typical per contact pair, 6μV max.

OFFSET CURRENT: <100pA.

**CONNECTOR TYPE:** 50 pin D-sub  $\times$  2.

RELAY DRIVE CURRENT: 20mA per channel.

ISOLATION BETWEEN ANY TWO TERMINALS:  $>10^{9}\Omega$ , <200pF.

ISOLATION BETWEEN ANY TERMINAL AND EARTH: >10  $^9\Omega,$  <400 pF.

CROSS TALK (1 MHz,  $50\Omega$  Load): <-40dB.

**INSERTION LOSS (50** $\Omega$  **Source, 50** $\Omega$  **Load):** <0.35dB below 1MHz.

<3dB below 2MHz.

COMMON MODE VOLTAGE: 300V between any terminal and chassis.


#### **ENVIRONMENTAL**

**OPERATING ENVIRONMENT:** Specified for 0°C to 50°C.

Specified to 40% R.H. at 35°C.

STORAGE ENVIRONMENT:  $-25^{\circ}\text{C}$  to  $65^{\circ}\text{C}$ .

WEIGHT: 0.8kg (1.75 lbs).

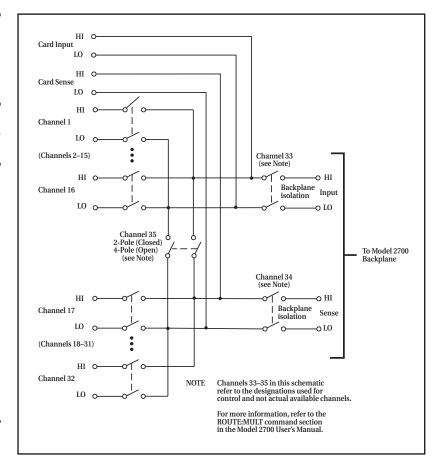





## Model 7700, 7702, and 7703 Multiplexer Modules

User's Guide

28775 Aurora Road Cleveland, Ohio 44139 (440) 248-0400 Fax: (440) 248-6168 www.keithley.com

## Introduction

WARNING

Connection and wiring procedures contained in this User's Guide are intended for use by qualified service personnel only. Do not perform these procedures unless qualified to do so. Failure to recognize and observe normal safety precautions could result in personal injury or death.

This document contains information specific to the Models 7700, 7702, and 7703 multiplexer modules. These modules can be used in the following Model 27xx DMM mainframes:

- 7700 Module This module can be used in Model 2700, 2701, and 2750 mainframes.
- 7702 Module This module can be used in Model 2700, 2701, 2750, and 2790 mainframes.
- 7703 Module This module can be used in Model 2700, 2701, and 2750 mainframes.

All references to the Model 27xx apply to the Models 2700, 2701, and 2750.

If you have any questions after reviewing this information, please contact your local Keithley representative or call our Applications Engineers at 1-888-KEITHLEY (1-888-534-8453, U.S. only) or Telefax: 440-498-2990 (Instrument Products).

WARNING

Before operating the Model 27xx with an accessory card, verify that the card is properly installed and the mounting screws are tightly fastened. If the mounting screws are not properly connected, an electrical shock hazard may be present.

## **Operation**

Model 7700 Operation of the Model 7700 module is covered in Section 2 of the Models 2700, 2701, and 2750 User's Manuals.

Model 7702 Except for the number of available switching channels and channel number designations, operation of the Model 7702 is the same as operation for the Model 7700. Model 7700 operation is covered in Section 2 of the Models 2700, 2701, and 2750 User's Manuals. Model 7702 operation is also covered in Section 2 of the Model 2790 Reference Manual and Section 3 of the Model 2790 User's Manual. Channel number designations for the Model 7702 is provided in the schematic provided at the beginning of this user's guide.

Model 7703 This module is also similar to the Model 7700. Differences include the number of available channels and the Model 7703 does support amps measurements. Model 7700 operation is covered in Section 2 of the Models 2700, 2701, and 2750 User's Manuals. Channel number designations for the Model 7703 are provided at the end of this User's Guide.

**Amps measurements** – The 7703 module does not support amps measurements. System channel operation cannot be used to close channels while an amps function (DCI or ICI) is selected. See the Model 27xx Manual for details.


- If an amps function (DCI or ACI) is selected and you attempt to close a system channel, the message "NO AMPS CHAN" will be displayed briefly. For remote programming, error -222 (Parameter data out of range) is generated.
- If a system channel is already closed and you attempt to select the DCI or ACI function, the message "INVALID FUNC" will be displayed briefly. For remote programming, error -221 (Settings conflict) is generated.

**Making amps measurements** – In order to perform amps measurements, you must use the front panel inputs of the 27xx mainframe. You can still use the 7703 module for other aspects of the test (such as controlling a bias supply for DUT), but you must use multiple channel operation to close channels.

## Screw terminal access (Model 7700 and 7702)

Turn the access screw to unlock and open the cover. Press in the access screw to lock.

Figure 1
Screw terminal access

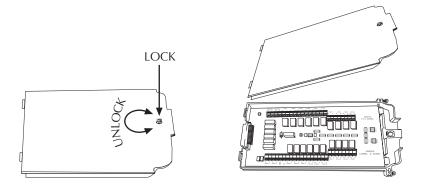

## Model 7700 - connections and wiring

The Model 7700 is a 20-channel differential multiplexer module with the following features:

- 2-wire or 4-wire  $\frac{3}{4}$  measurement (automatically pairs switches for four wire measurements n + 10)
- Screw terminal connections
- Temperature applications (RTD, thermistor, thermocouple)
- Two protected channels for current measurements (external shunts not required)
- Built-in cold junction reference
- Latching type relays (relays hold their position after power is removed)
- Designed specifically for use with Keithley's Models 2700, 2701, and 2750 Systems.

### **Connection information**

WARNING The information in this section is intended for qualified service personnel. Do not attempt to perform this procedure unless qualified to do so.


Do not exceed the maximum specifications for the Model 7700.

Connections to DMM functions are provided through the card backplane connector.

- Current provided for through two protected channels (Channels 21 and 22).
- INPUT connections.
- SENSE (3/44 Wire) connections.
- AMP and LO common connections to the DMM are also provided.

Figure 2

Model 7700 screw terminal channel designations

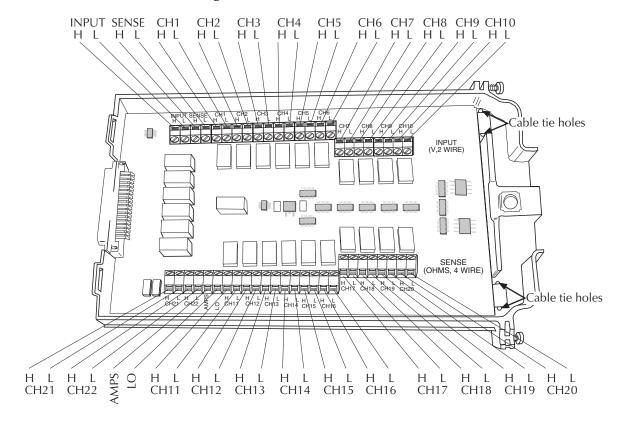

### Wiring procedure


WARNING The information in this section is intended for qualified service personnel. Do not attempt to perform this procedure unless qualified to do so.

Use the following procedure to wire the Model 7700 module. Make all connections using correct wire size (up to 20 AWG). Also, make sure to add supplementary insulation around the harness for voltages above 42V peak (see Figure 3).

WARNING All wiring must be rated for the maximum voltage in the system. For example, if 1000V is applied to the front terminals of the Models 2700, 2701, or 2750, the plug-in module wiring must be rated for 1000V.

- 1. Make sure all power is discharged from the Model 7700 module.
- 2. Access the screw terminals (see "Screw terminal access" located at the front of this document).
- 3. Using a small flat-blade screwdriver, loosen terminal screws and install wires as desired. (Figure 3 shows connections to channels 1 and 2).
- 4. Route wire along wire-path and secure with cable tie as shown.
- 5. Fill in a copy of the connection log and affix it to the module cover.
- 6. Close and lock the cover.

Figure 3
Wire dressing — Model 7700

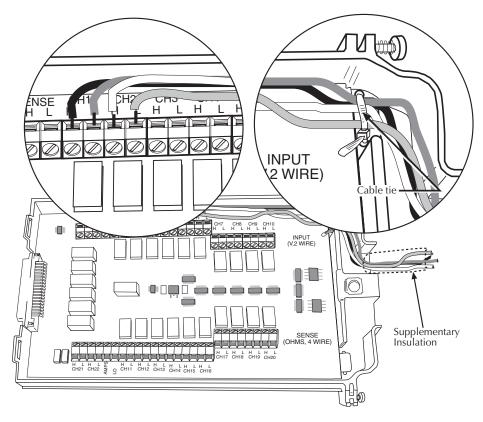

### **Connection log**

Make a copy of Table 1 and affix it to the cover of the Model 7700. Use this to record connection information and channel descriptions as needed.

Table 1 **Connection log Model 7700** 

Channel		Color	Description
AMPS COM	Н		
AMISCOM	L		
INPUT	Н		
INIOI	L		
SENSE	Н		
	L		
	Н		
CH1	L		
CHA	Н		
CH2	L		
	Н		
CH3	L		
	Н		
CH4	L		
	Н		
CH5	L		
	H		
CH6	L		
	H		
CH7	L		
CH8	Н		
	L		
CH9	Н		
	L		
CH10	Н		
01110	L		
CH11	Н		
CIIII	L		
CH12	Н		
CIIIZ	L		
CH12	Н		
CH13	L		
CILLA	Н		
CH14	L		
GTT1 5	Н		
CH15	L		
	Н		
CH16	L		
	Н		
CH17	L		
	H		
CH18	L		
	H		
CH19	L		
CH20	Н		
	L		
AMPS21	Н		
	L		
AMPS22	Н		
	L		

## Model 7702 – connections and wiring

The Model 7702 is a 40-channel differential multiplexer module with the following features:

- 2-wire or 4-wire  $\frac{3}{4}$  measurement (automatically pairs switches for four wire measurements n + 20)
- Two protected channels for current measurements (external shunts not required)
- Temperature applications (RTD, thermistor, thermocouple)
- Latching type relays (relays hold their position after power is removed)
- · Screw terminal connections
- Designed specifically for use with Keithley's Models 2700, 2701, 2750 or 2790 Systems.

#### **Connection information**

**WARNING** 

The information in this section is intended for qualified service personnel. Do not attempt to perform this procedure unless qualified to do so.

Do not exceed the maximum specifications for the Model 7702.

Connections to DMM functions are provided through the card backplane connector.

- Current provided for through two protected channels (Channels 41 and 42).
- INPUT connections.
- SENSE (3/44 Wire) connections.
- AMP and LO common connections to the DMM are also provided.

### Wiring procedure

WARNING

The information in this section is intended for qualified service personnel. Do not attempt to perform this procedure unless qualified to do so.

Use the following procedure to wire the Model 7702 module. Make all connections using correct wire size (up to 20 AWG). Also, make sure to add supplementary insulation around the harness for voltages above 42V peak (see Figure 5).

WARNING All wiring must be rated for the maximum voltage in the system. For example, if 1000V is applied to the front terminals of the Models 2700, 2701, 2750, or 2790, the plug-in module wiring must be rated for 1000V.

- 1. Make sure all power is discharged from the Model 7702 module.
- 2. Access the screw terminals (see "Screw terminal access" located at the front of this document).
- 3. Using a small flat-blade screwdriver, loosen terminal screws and install wires as desired. (Figure 5 shows connections to the Input and Sense).
- 4. Route wire along wire-path and secure with cable ties as shown.
- 5. Fill in a copy of the connection log and affix it to the module cover.
- 6. Close and lock the cover.

Figure 4

Model 7702 Screw terminal channel designations


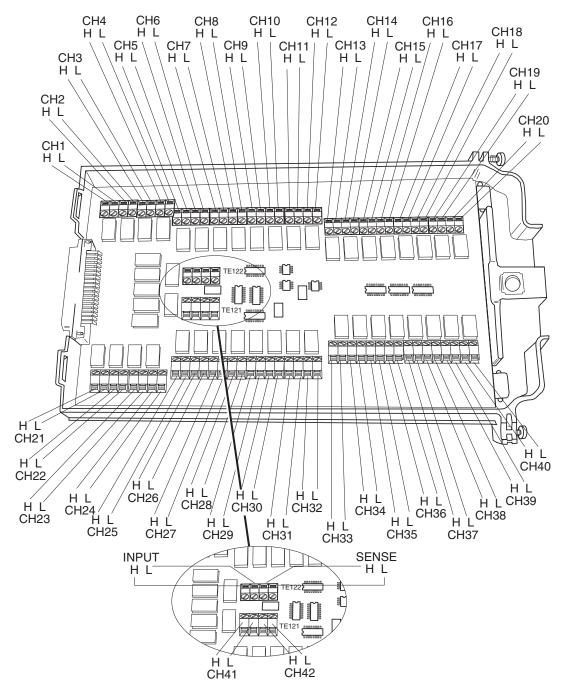


Figure 5
Wire dressing — Model 7702

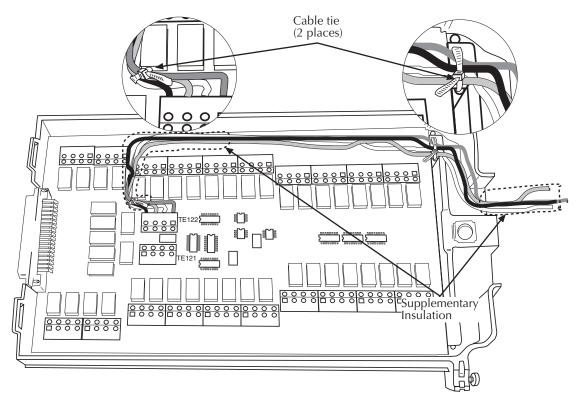

## **Connection log**

Make a copy of Table 2 and affix it to the cover of the Model 7702. Use this to record connection information and channel descriptions as needed.

Table 2 **Connection log Model 7702** 

Channel			Description	Color	Channel		
INPUT	Н			-			
	L H			-			
SENSE	L			-			
СПО	Н					Н	CH1
CH21	L					L	СПІ
CH22	Н					Н	CH2
	L H					L H	
CH23	L			-		L	CH3
	Н					Н	
CH24	L			-		L	CH4
CH25	Н					Н	CH5
CH23	L			-		L	СПЭ
CH26	Н					Н	СН6
	L					L	
CH27	H L			-		H	CH7
	Н					H	
CH28	L			-		L	CH8
GHOO	Н					Н	CHO
CH29	L					L	CH9
CH30	Н					Н	CH10
C1130	L					L	,
CH31	Н			-		Н	CH11
	L H					L H	
CH32	L					L	CH12
	Н					Н	
CH33	L					L	CH13
CH34	Н					Н	CH14
C1134	L					L	CIII4
CH35	Н					Н	CH15
	L					L	
CH36	H			H	CH16		
	Н					H	
CH37	L					L	CH17
CH38	Н					Н	СП10
	L			1		L	CH18
CH39	Н					Н	CH19
	L					L	
CH40	Н					Н	CH20
	L					L H	
AMPS41	L					L	AMPS42
			L				

## Model 7703 – connections and wiring

The Model 7703 is a 32-channel high speed differential multiplexer module with the following features:

- 2-wire or 4-wire  $\frac{3}{4}$  measurement (automatically pairs switches for four wire measurements n + 16)
- 50-pin D-Shell connectors (2 × DB50)
- Temperature applications (RTD or thermistor)
- High-speed non-latching reed relays (relays go to open state after power is removed or \*RST)
- Designed specifically for use with Keithley's Models 2700, 2701, and 2750 Systems.

NOTE The 50-pin D-Shell connector mates with Model 7788.


### **Card configuration—connections**

WARNING The information in this section is intended for qualified service personnel. Do not attempt to perform this procedure unless qualified to do so.

Do not exceed the maximum specifications for the Model 7703 module.

NOTE When looking at the rear connectors of the Model 7703 module, the connector on the left is P1017 and the connector on the right is P1016.

Figure 6
Rear view—Model 7703 Pinouts (P1016 and P1017)




Make all connections using correct wire size (up to 20 AWG). Also, make sure to add supplementary insulation around the harness for voltages above 42V peak (see Figure 7).

WARNING All wiring must be rated for the maximum voltage in the system. For example, if 1000V is applied to the front terminals of the Models 2700, 2701, or 2750, the plug-in module wiring must be rated for 1000V.

Make all connections using correct wire size (up to 20 AWG) (refer to the Model 7788 documentation for specific wiring instructions).

CAUTION If both connectors (P1017 and P1016) are not used, install the extra Model 7788 50-pin D-shell as a plug on the open connector (see Figure 7). If the connector is left open, an electrical shock hazard may be present.

Figure 7
Supplementary insulation and plugging an unused connector

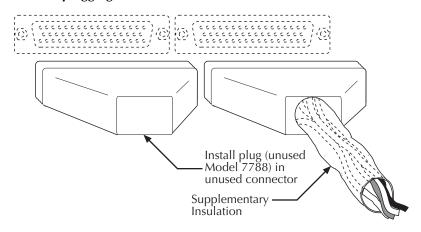

*Table 3* **Model 7703 channel designations** 

P1017							
Pin	СН	Pin	СН	Pin	СН		
18	9 HI	30	15 HI	42	29 HI		
19	9 LO	31	15 LO	43	29 LO		
20	10 HI	32	16 HI	44	30 HI		
21	10 LO	33	16 LO	45	30 LO		
22	11 HI	34	25 HI	46	31 HI		
23	11 LO	35	25 LO	47	31 LO		
24	12 HI	36	26 HI	48	32 HI		
25	12 LO	37	26 LO	49	32 LO		
26	13 HI	38	27 HI				
27	13 LO	39	27 LO				
28	14 HI	40	28 HI				
29	14 LO	41	28 LO				

P1016								
Pin	СН	Pin	СН	Pin	СН			
1	Sense HI	26	5 HI	38	19 HI			
2	Sense LO	27	5 LO	39	19 LO			
4	Input HI	28	6 HI	40	20 HI			
6	Input LO	29	6 LO	41	20 LO			
18	1 HI	30	7 HI	42	21 HI			
19	1 LO	31	7 LO	43	21 LO			
20	2 HI	32	8 HI	44	22 HI			
21	2 LO	33	8 LO	45	22 LO			
22	3 HI	34	17 HI	46	23 HI			
23	3 LO	35	17 LO	47	23 LO			
24	4 HI	36	18 HI	48	24 HI			
25	4 LO	37	18 LO	49	24 LO			

### **Connection log**

Make a copy of Table 4 and affix it to the cover of the Model 7703. Use this to record connection information and channel descriptions as needed.

Table 4 **Connection log Model 7703** 

NPUT   L	Channel		Color	Description	Description	Color	Cha	annel
SENSE	INPUT	Н						
SENSE         L         H         H         CH17           CH1         H         L         CH17           CH2         H         H         CH18           CH3         H         H         CH19           CH4         H         CH19         CH19           CH4         H         CH20         CH20           CH5         H         H         CH21           CH6         H         H         CH21           CH7         H         H         CH22           CH7         H         H         CH23           CH8         H         H         CH24           CH8         H         H         CH24           CH9         H         CH24         CH24           CH10         H         H         CH25           CH11         H         CH26         CH27           CH12         H         CH27         CH28           CH13         H         H         CH29           CH14         H         H         CH30           CH15         H         H         CH31           CH16         H         CH31         CH31 <td>111101</td> <td>L</td> <td></td> <td></td> <td></td> <td></td> <td></td> <td></td>	111101	L						
CH1	SENSE -	Н						
CH1		L						
CH2	CH1	Н					Н	CH17
CH2  CH3  H  CH4  H  CH4  H  CH5  H  CH6  H  CH6  H  CH7  CH7  H  CH7  CH7		L					L	CIII
CH3	CH2	Н						CH18
CH3  L CH4  H L CH5  H L CH5  H CH6  H L CH6  H L CH7  CH7  H L CH7  CH7  H CH7  CH8  H CH7  CH8  CH9  H CH7  CH9  H CH7  CH9  H CH7  CH9  CH9	C112	L					L	CIIIO
CH4       H       H       CH20         CH5       H       H       CH21         CH6       H       H       CH21         CH6       H       H       CH22         CH7       H       H       CH23         CH8       H       H       CH24         CH9       H       H       CH24         CH10       H       H       CH25         CH11       H       H       CH26         CH12       H       H       CH27         CH13       H       H       CH28         CH14       H       H       CH30         CH15       H       H       CH31         CH16       H       CH31       H         CH16       H       CH31       H	CH3	Н						CH19
CH4  L  CH5  H  CH6  H  CH6  L  CH7  H  CH7  CH7  CH7  CH8  H  CH8  CH9  CH9  CH9  CH10  H  CH10  CH10	CHS	L					L	CIII)
CH5	CH4	Н					Н	CH20
CH5	CITT	L					L	C1120
CH6	CH5	Н					Н	CH21
CH6         L         CH22           CH7         H         H         CH23           CH8         H         L         L         CH24           CH9         H         H         CH24         CH24           CH9         H         H         CH25         CH25           CH10         H         H         CH26         CH26           CH11         H         CH26         CH27         CH27           CH12         H         H         CH28         CH28           CH13         H         H         CH29         CH29           CH14         H         H         CH30         CH30           CH15         H         H         CH31         CH31           CH16         H         H         CH32	CHS	L					L	CHZI
CH7	CH6	Н					Н	CH22
CH7  L  CH8  H  L  CH9  H  CH9  H  CH10  H  CH10  H  CH10  H  CH11  L  CH12  CH11  CH12  H  CH12  CH12  CH11  CH12  H  CH12  CH12  CH13  H  CH13  CH14  CH15  H  CH23  CH24  CH24  CH24  CH25  CH25  CH25  CH25  CH26  CH26  CH26  CH27  CH26  CH27  CH27  CH27  CH27  CH28  CH28  CH28  CH28  CH30  CH30  CH30  CH30  CH31  CH31  CH31	CHO	L					L	CHZZ
CH8	CH7	Н					Н	CH23
CH8       L       L       CH24         CH9       H       H       H       CH25         CH10       H       H       CH26         CH11       H       CH26       CH26         CH11       H       CH27       CH27         CH12       H       H       CH28         CH13       H       H       CH29         CH14       H       H       CH30         CH15       H       H       H       CH31         CH16       H       CH32	CIII	L					L	C1123
CH9	СПб	Н					Н	СПЭЛ
CH9  L  CH10  H  CH10  L  CH11  H  CH26  CH11  L  CH27  CH12  H  CH27  CH12  H  CH28  CH13  H  CH28  CH13  H  CH29  CH14  H  CH30  CH15  H  CH31  CH16	CHO	L					L	C1124
CH10	СПО	Н					Н	CU25
CH10  L CH26  CH11  H CH27  CH12  H CH28  CH12  H CH28  CH13  H CH28  CH14  H CH29  CH14  H CH30  CH15  H CH31  CH16	CH	L					L	CH25
CH11	CH10	Н					Н	СПЗЕ
CH11     L     CH27       CH12     H     H     CH28       CH13     H     H     CH29       CH14     H     H     CH30       CH15     H     H     H     CH31       CH16     H     CH32	CITIO	L					L	СП20
CH12	CHILL	Н					Н	CHOT
CH12  L CH28  CH13  H CH29  CH14  H CH29  CH14  L CH30  CH15  H CH31  CH16	СПП	L					L	СП21
CH13	CH12	Н					Н	CH28
CH13  L CH29  CH14  H CH30  CH15  H CH30  CH15  H CH31  CH16	CHIZ	L					L	
CH14     H     H     CH30       CH15     H     H     CH31       CH16     H     CH32	СП13	Н					Н	CHOO
CH14         L         CH30           CH15         H         H         CH31           CH16         H         H         CH32	СПІЗ	L					L	СП29
CH15	CH14	Н					Н	CH20
CH15 L CH31  CH16 H CH32		L					L	CH3U
CH16 H CH32	CH15	Н					Н	CH31
CH16 CH32	CHIS	L					L	
CHIO L CH32	CH16	Н					Н	CHOO
		L					L	CH32

Specifications are subject to change without notice.

All Keithley trademarks and trade names are the property of Keithley Instruments, Inc.

All other trademarks and trade names are the property of their respective companies.



A GREATER MEASURE OF CONFIDENCE

### **Keithley Instruments, Inc.**

Corporate Headquarters • 28775 Aurora Road • Cleveland, Ohio 44139 • 440-248-0400 • Fax: 440-248-6168 • 1-888-KEITHLEY (534-8453) • www.keithley.com