

MODEL 552G OSCILLOSCOPE

OPERATION MANUAL

印刷表紙使用の巻と

KIKUSUI ELECTRONICS CORP.

Contents

	Page
General	3
Specifications	4
Front Panel	7
Rear Panel	11
Operating Procedure	13
Measuring Procedure	15
1. Measurement of phase difference	15
2. Frequency measurement	17
Maintenance	19
Adjustment of vertical axis DC balance	19
Adjustment of horizontal axis DC balance	20
Adjustment of astigmatism	21
Removal of case	21
Adjustment of power voltage	23
Adjustment of CAL mV_{p-p} (calibration voltage)	24
Adjustment of trace center	24

General:

Kikusui Electronics' Model 552G is an x-y oscilloscope to be used in combination with a sweep generator for direct-viewing the frequency response of measuring instruments. The 552G is designed to be compact by using a cathode-ray tube 133 mm in screen diameter. The circuitry uses semi-conductors to the full extent, and balanced DC amplifiers of high sensitivity and stability. Compared with the vacuum-tube oscilloscope, the 552G has less drift and higher reliability.

Provided with a line sweep, the 552G is suitable for use in a mass-production line which employs a concentrated type sweep generator. Also, the 552G is widely usable as it includes a high-sensitivity z-axis (intensity modulation) terminal and a sensitivity calibration voltage of stabilized square wave.

Specifications:

Power Requirements	-----V, 50 or 60 Hz, approx. 30 VA
Dimensions (maximum)	164 mm wide, 254 (280) mm high, 405 (445) mm deep
Weight	Approx. 18 kg
Vertical Axis	
Sensitivity	More than 10 mV _{p-p} /cm More than 100 mV _{p-p} /cm with the voltage divider set to 1/10 More than 1 V _{p-p} /cm with the voltage divider set to 1/100 Sensitivity is continuously variable down to approx. 1/10 with the VARIABLE knob.
Voltage Dividing Accuracy	Within ± 0.5 dB
Frequency Response	AC Less than -3 dB at 2 Hz to 500 kHz DC Less than -3 dB at 0 to 500 kHz
Input Impedance	Approx. 1 M Ω ; parallel capacitance, 50 \pm 1.5 pF
Input Terminal	UHF-type receptacle (also appli- cable to M-type)
Allowable Input Voltage	600 V (peak value including DC component)

Horizontal Axis

Sensitivity	More than 200 mV/cm
Frequency Response	AC Less than -3 dB at 2 Hz to 50 kHz DC Less than -3 dB at 0 to 50 kHz
Input Impedance	Approx. 220 k Ω ; parallel capacity, less than 30 pF
Input Terminal	Binding post
Allowable Input Voltage	100 V (peak value including DC component)
Line Sweep Built In	Phase variation range: Approx. 130 $^{\circ}$
Calibration Voltage	
Output Voltage	10, 20 and 50 mV _{p-p} square waves
Accuracy	$\pm 5\%$

Miscellaneous

Cathode-ray Tube	5UPIF
Acceleration Voltage	Approx. 1300 V
Effective Screen Area	8 x 10 cm

Accessories


Model 941B Terminal Adapter	1
Short Bar	1
Operation Manual	1
Test Data	1

Intensity Modulation

System	Z-axis intensity modulation
--------	-----------------------------

Sensitivity	Sufficient modulation obtained with 1 V _{p-p} signal
Frequency Response	Less than -3 dB at 100 Hz to 400 kHz
Input Impedance	Approx. 220 k Ω ; parallel capacitance, less than 60 pF
Polarity of Modulation	Brightness increases with positive signal.
Miscellaneous	Since a limiter is provided, nearly constant modulation is applied. Usable within a range of 1 - 10 V _{p-p} without adjustment.
Allowable Input Voltage	100 V (peak value including DC component)

Front Panel:

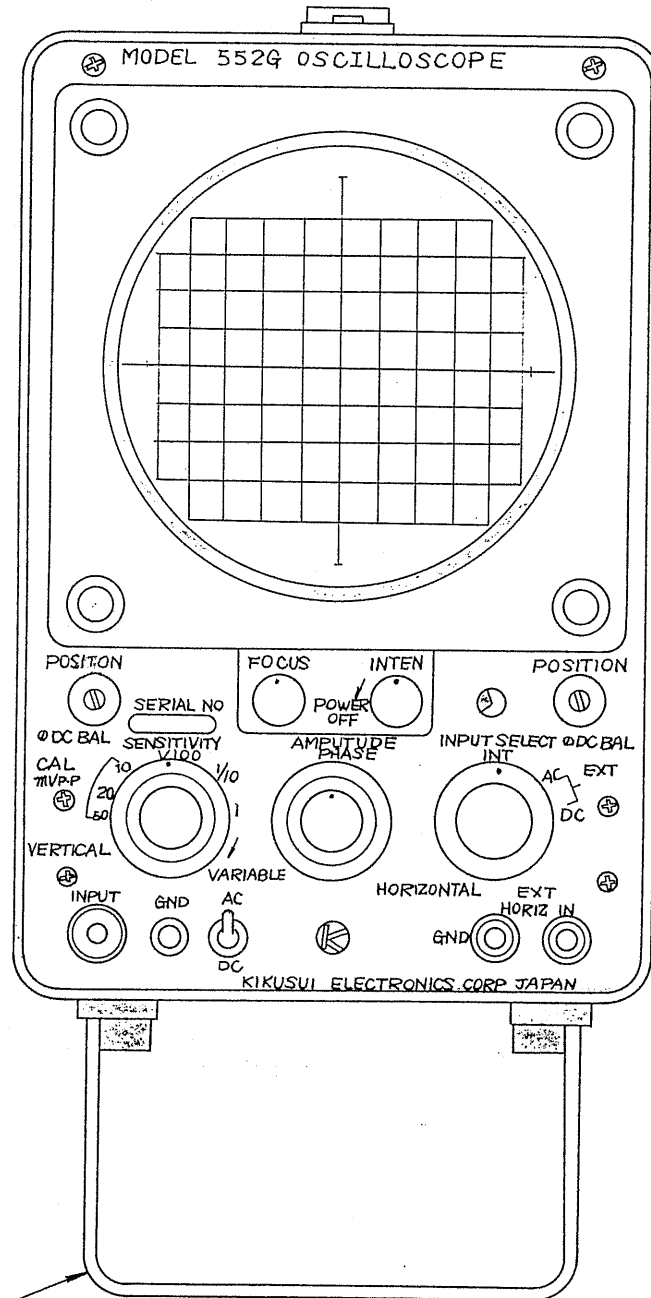

Stand

POWER OFF When this knob is turned full
 counterclockwise, power supply turns off.

 When turned clockwise from the above position,
 the knob clicks. Then power supply turns on,
 and the pilot lamp (neon) on the right side of
 the knob lights. This knob is also used for
 INTENSITY control..

INTEN Knob for controlling the brightness on CRT.

 As the knob is turned clockwise, the brightness
 increases. This knob is also used as the power
 switch.

FOCUS Knob for adjusting the focus on CRT. Turn the
 knob so that the trace becomes most clear
 and sharp.

VERTICAL

POSITION Knob for adjusting the trace position
 vertically.

DC BAL Screw located at the center of the POSITION
 knob. A semi-fixed variable resistor is
 provided for adjusting the DC balance of the
 vertical axis amplifier. Use a screwdriver
 for adjustment. Refer to "Adjustment of
 vertical axis DC balance," page 19..

INPUT Terminal for vertical axis input.

AC and DC Switch for changing over the vertical axis
 input to AC or DC coupling.

SENSITIVITY Outer black knob for selecting 1, 1/10 or 1/100 sensitivity by the input voltage divider of the vertical axis amplifier. When the knob is set to CAL 10, 20 or 50 mV_{p-p} position, the sensitivity calibration voltage inside the equipment is connected to the amplifier, and the sensitivity can easily be calibrated by using the VARIABLE knob.

VARIABLE Red knob for finely adjusting the sensitivity of the vertical axis amplifier. The sensitivity can be continuously adjusted to approximately 1/10.

HORIZONTAL POSITION Knob for adjusting the trace position horizontally.

DC BAL Screw located at the center of the POSITION knob. A semi-fixed variable resistor is provided for adjusting the DC balance of the horizontal axis amplifier. Use a screwdriver for adjustment. Refer to "Adjustment of horizontal axis DC balance," page.19.

EXT HORIZ IN Terminal for the external signal input for horizontal axis.

INPUT SELECT Switch for selection of internal or external

(AC or DC) horizontal axis input.


INT When the switch is set to this position, the horizontal axis input is connected to the line sweep inside the equipment.

EXT (AC/DC) Horizontal axis input is connected to the external input terminal. AC or DC coupling can further be selected.

AMPLITUDE Outer black knob for adjusting the sensitivity of the horizontal axis amplifier. The sensitivity can be continuously adjusted to approximately 1/10.

PHASE Red knob for adjusting the phase of internal line sweep. The phase is continuously adjustable from 0 to approximately 130° .

Rear Panel:

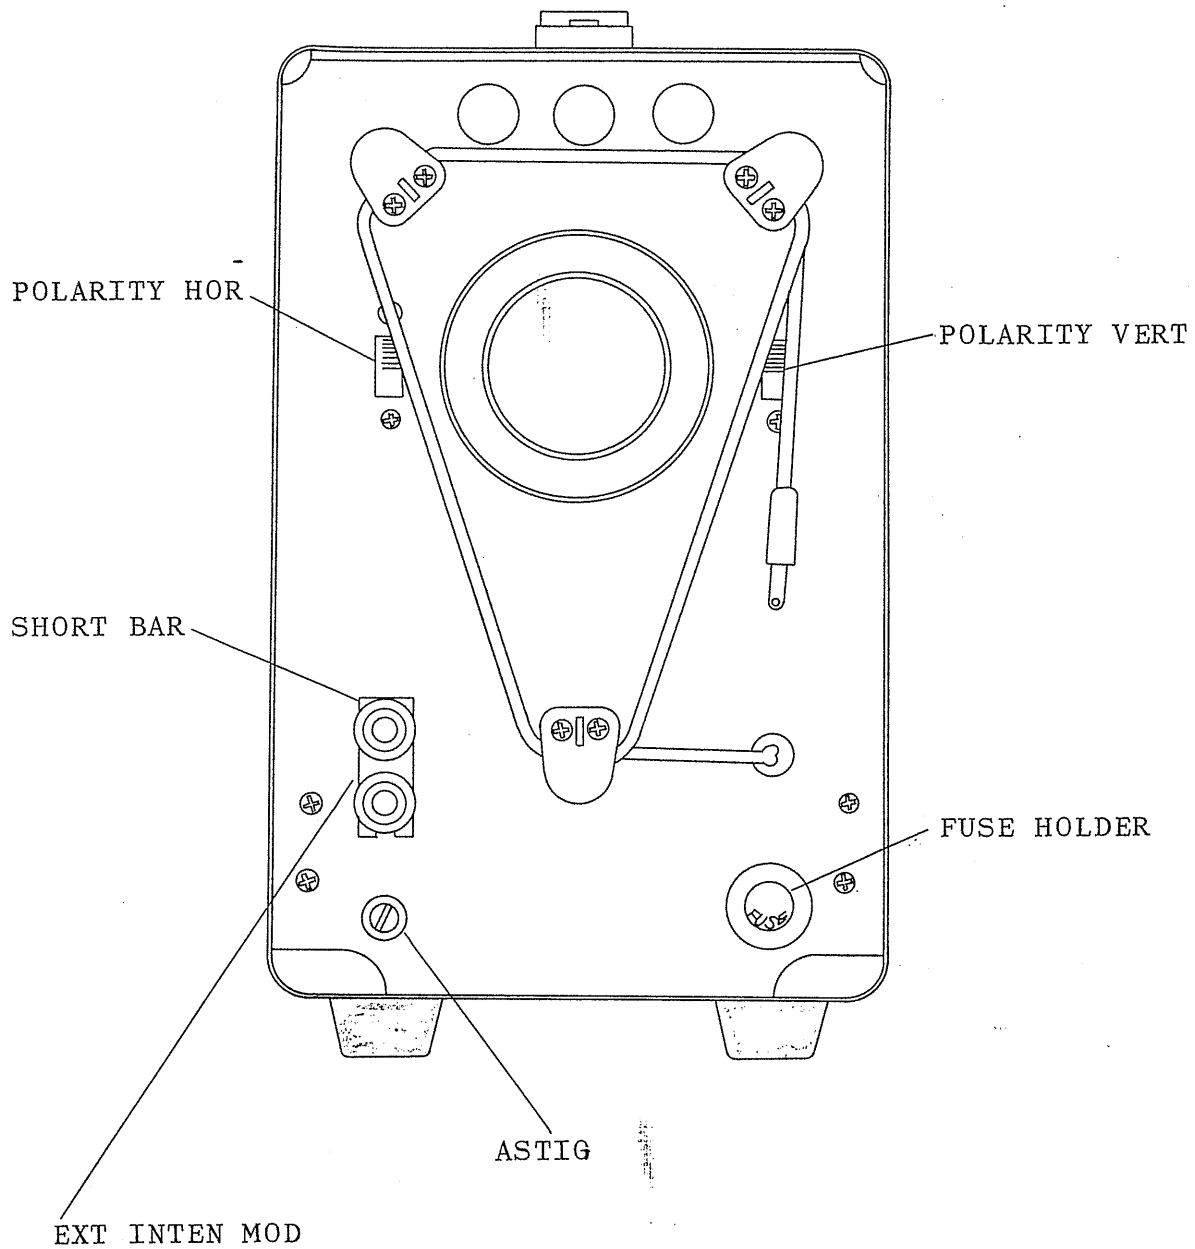

POLARITY VERT

Switch for changing over the polarity of vertical axis. Set the switch to the lower position when desiring to reverse the polarity of trace waveform 180° vertically. For normal operation, keep the switch set to the upper position.

POLARITY HOR

Switch for changing over the polarity of horizontal axis. Set the switch to the lower position when desiring to reverse the polarity of trace waveform 180° horizontally. For normal operation, keep the switch set to the upper position.

EXT INTEN MOD

Terminals for z-axis intensity modulation input. The red terminal is for input application; the black terminal, for grounding. Input impedance is approximately $220\text{ k}\Omega$. When using the terminals, remove the short bar.

ASTIG

A semi-fixed variable resistor. For adjustment, refer to "Adjustment of astigmatism," page 20.

FUSE HOLDER

A one-ampere fuse is contained.

Operating Procedure:

- Line Voltage The 552G stably operates within a line voltage range of AC _____V. $\pm 10\%$. For the maximum reliability and part life, use the 552G at a line voltage as close to the center of the above voltage range as possible.
- Installation Install the 552G where the ambient temperature is within a range of 0 to 40° C. Keep it from direct sunlight, moisture and dust. When using it near the equipment, machine or other object which generates heat, consider appropriate ventilation.
- Other Cautions If there is a strong magnetic field nearby, the electron beam in the CRT may be abnormally deflected by the field. Also, noise may be picked up, and the trace distorted. Avoid using the 552G where corrosive gas exists. Such gas greatly shortens the life of electronic parts in the 552G.
- Allowable Input Voltage Do not apply voltages in excess of the maximum values listed below, to the vertical axis and horizontal axis input terminals. When a voltage higher than the maximum value

is applied, the input attenuator and other parts may be damaged.

Vertical axis input terminal: 600 V at maximum (peak value including DC component)


Horizontal axis input terminal: 100 V at maximum (peak value including DC component)

Use of EXT INTEN Remove the short bar from the EXT INTED MOD MOD (z-axis terminals located on the rear panel, and intensity apply intensity modulation signal there. modulation) The input voltage needed for modulation is terminals $1 V_{p-p}$ or more. The voltage may be pulse or sine wave, and the waveform polarity may be either positive or negative. Adjust the INTEN knob a little for the best modulation and image clearness.


1. Measurement of phase difference

The phase difference between two signals of the same frequency is measured by utilizing a Lissajous figure. Before starting this measurement, measure the intrinsic phase difference existing between the vertical and horizontal amplifiers in the 552G since such phase difference cannot be neglected at certain frequencies.

Set the HORIZONTAL INPUT SELECT switch to the EXT AC or DC position, apply the sine wave output of a low-frequency signal generator to the vertical and horizontal input terminals as illustrated below, and measure the intrinsic phase difference of the 552G.

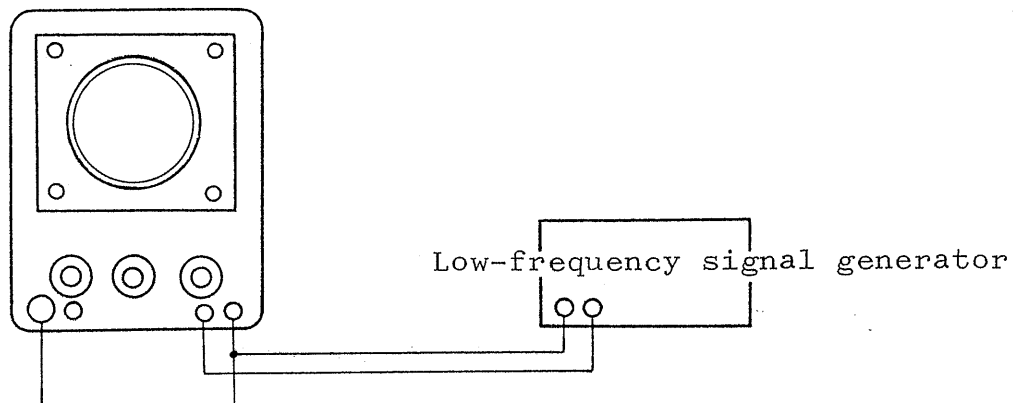


Adjust the SENSITIVITY switch, and VARIABLE AND AMPLITUDE knobs so that a figure of appropriate size is traced on the screen as shown below. Vary the frequency of the low-frequency signal generator, then a loop figure will be formed as shown at a frequency of several tens of kilohertz.

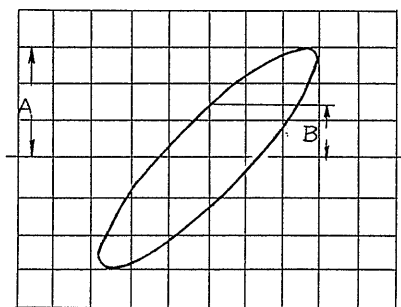

The intrinsic phase difference can be obtained as follows:
Set the horizontal and vertical amplitudes of the loop figure to the scale as shown above, read values A and B, and calculate the phase difference angle by using the following formula:


$$\text{Phase difference angle} = \sin^{-1} \frac{B}{A}$$

This phase difference angle measuring method can be applied to, for example, the measurement of phase difference between input and output of an amplifier, as illustrated below. The true phase difference is the intrinsic phase difference angle of the amplifier subtracted from the phase difference angle measured.

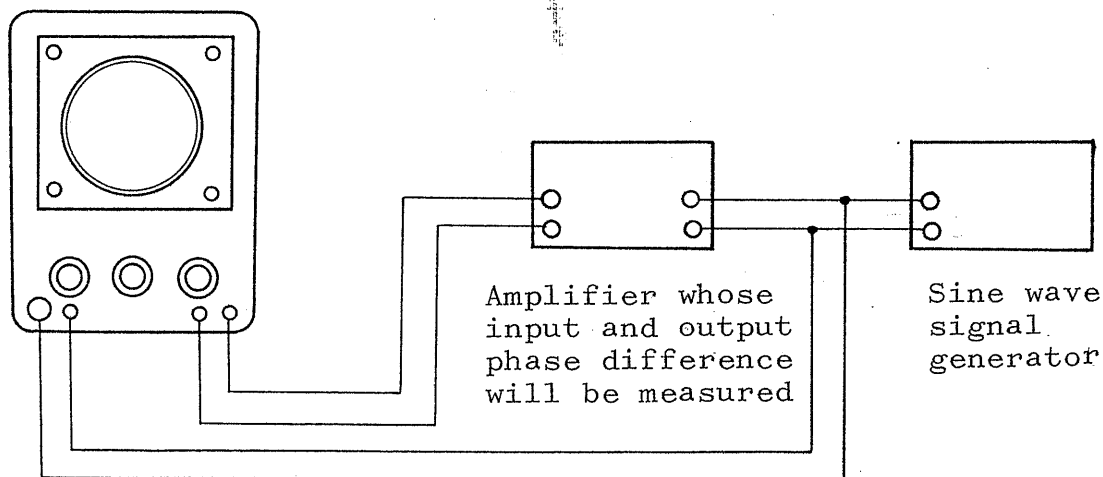

2. Frequency measurement

A Lissajous figure can be obtained on the CRT when two kinds of AC voltages are applied to the vertical and horizontal axes simultaneously. By utilizing the figure and a known reference frequency, the unknown frequency of the signal applied can be measured. A connection diagram for this measurement is shown below:






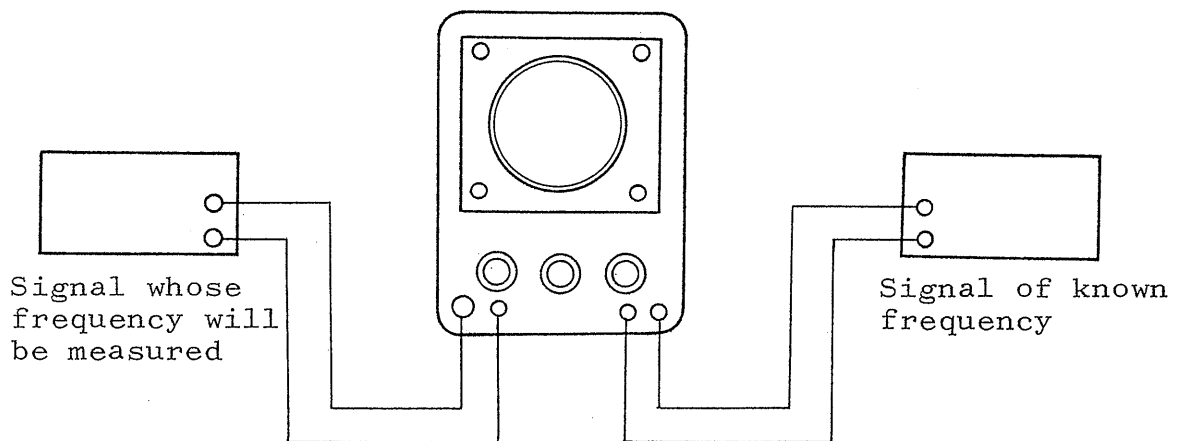


When the ratio of vertical frequency to horizontal frequency is integral in value, the figure on CRT stops showing one of the patterns illustrated below.

Count the number (NV) of hte points where the loop is in contact with vertical tangents, and the number (Nh) of the points where the loop is in contact with horizontal tangents. Then the vertical and horizontal input frequencies fV and fh can be obtained by using the following formula:

$$\frac{fV}{fh} = \frac{Nh}{NV}$$

Two different values may be obtained for N_V and N_h , respectively, depending on the phase relationship between the two signals, as shown below. The figures in the upper row and the figures immediately below them correspond to each other, respectively.



$$\frac{f_V}{f_n} = \frac{3}{2}$$

$$\frac{f_V}{f_n} = \frac{4}{3}$$

$$\frac{f_V}{f_n} = \frac{2}{1}$$

Maintenance:


Adjustment of vertical axis DC balance

Conduct this adjustment 15 to 20 minutes after the 552G is energized.

1. Short the vertical input and GND terminals between them.
2. Turn the SENSITIVITY VARIABLE knob full counterclockwise, and set the trace to the center of the scale by turning the vertical POSITION knob.
3. Turn the VARIABLE knob full clockwise. If the trace shifts upward or downward when the knob is thus turned, vertical DC balance is maladjusted.

Correct the DC balance as follows:

4. Leave the VARIABLE knob turned full clockwise, and turn the DC BAL screw with a screwdriver to adjust the trace to the center of the scale.
5. Turn the VARIABLE knob full clockwise and counterclockwise alternately. If the trace still shifts then, finely adjust the DC BAL screw. Repeat the above adjusting procedure until the trace does not shift when the VARIABLE knob is turned.

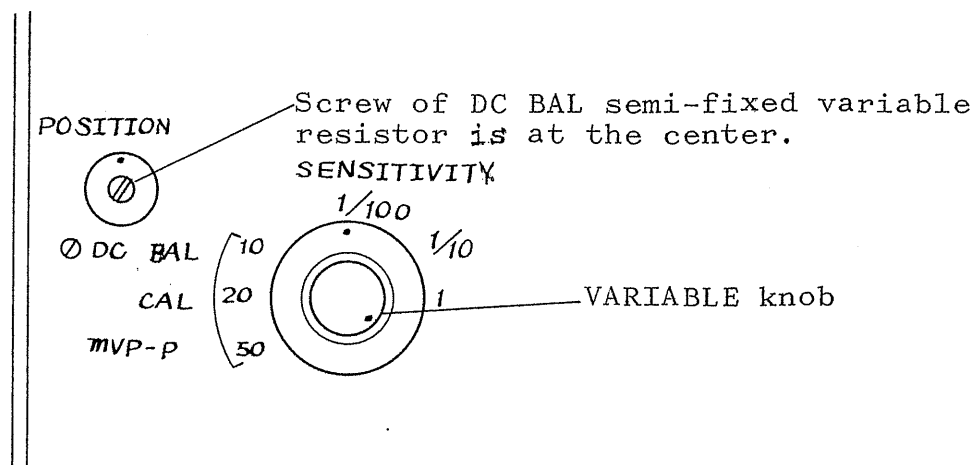


Adjustment of horizontal axis DC balance

Conduct this adjustment 15 to 20 minutes after the 552G is energized.

1. Short the horizontal input and GND terminals between them, and set the INPUT SELECT switch to EXT AC or DC.
2. Turn the AMPLITUDE knob full counterclockwise, and set the trace to the center of the scale by turning the horizontal POSITION knob.
3. Turn the AMPLITUDE knob full clockwise. If the trace shifts rightward or leftward when the knob is thus turned, horizontal DC balance is maladjusted.

Correct the DC balance as follows:

4. Leaving the AMPLITUDE knob turned full clockwise, turn the DC BAL screw with a screwdriver to adjust the trace to the center of the scale.
5. Turn the AMPLITUDE knob full clockwise and counterclockwise alternately. If the trace still shifts then, finely adjust the DC BAL screw. Repeat the above adjusting procedure until the trace does not shift when the AMPLITUDE knob is turned.

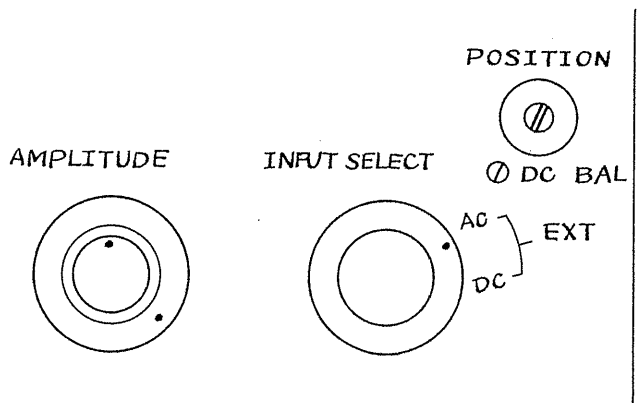

Adjustment of astigmatism

Conduct this adjustment with the ASTIG semi-fixed variable resistor located on the rear panel.

1. Let the 552 G trace a waveform.
2. Adjust the ASTIG screw and the FOCUS knob on the front panel so that the trace has a uniform thickness over the entire scale and has the highest sharpness and clearness.

Removal of case

Remove the two screws located on both sides, respectively, of the equipment case, and the screw located on the bottom.

(Locations of the screws are illustrated below.)


Then gently pull out the front panel and chassis together.

Be sure to deenergize the 552G before removing the case, since high voltages are exposed at various points in the equipment.

Two screws on
this side -

Screw on bottom

Two screws
on this
side

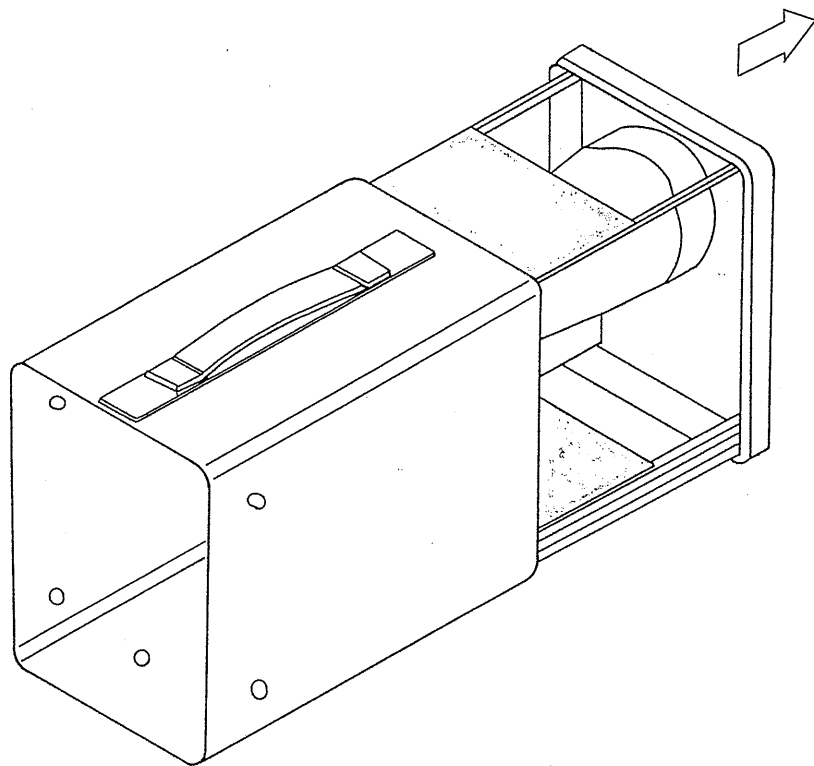


Adjustment of power voltage

Two power supply systems for regulated +12 and -9 V are provided as shown in the attached drawing "Power Supply and CRT Circuit."

The +12 V is adjustable with semi-fixed resistor R318.

Although a semi-fixed resistor is not provided for adjustment of the -9 V, this voltage is automatically set to approximately -9 V when the +12 V is adjusted. The location of semi-fixed resistor R318 is shown below.

For checking output voltage, measure the voltage between the test point marked "+12 V" or "-9 V" on the printed circuit board, and the ground.

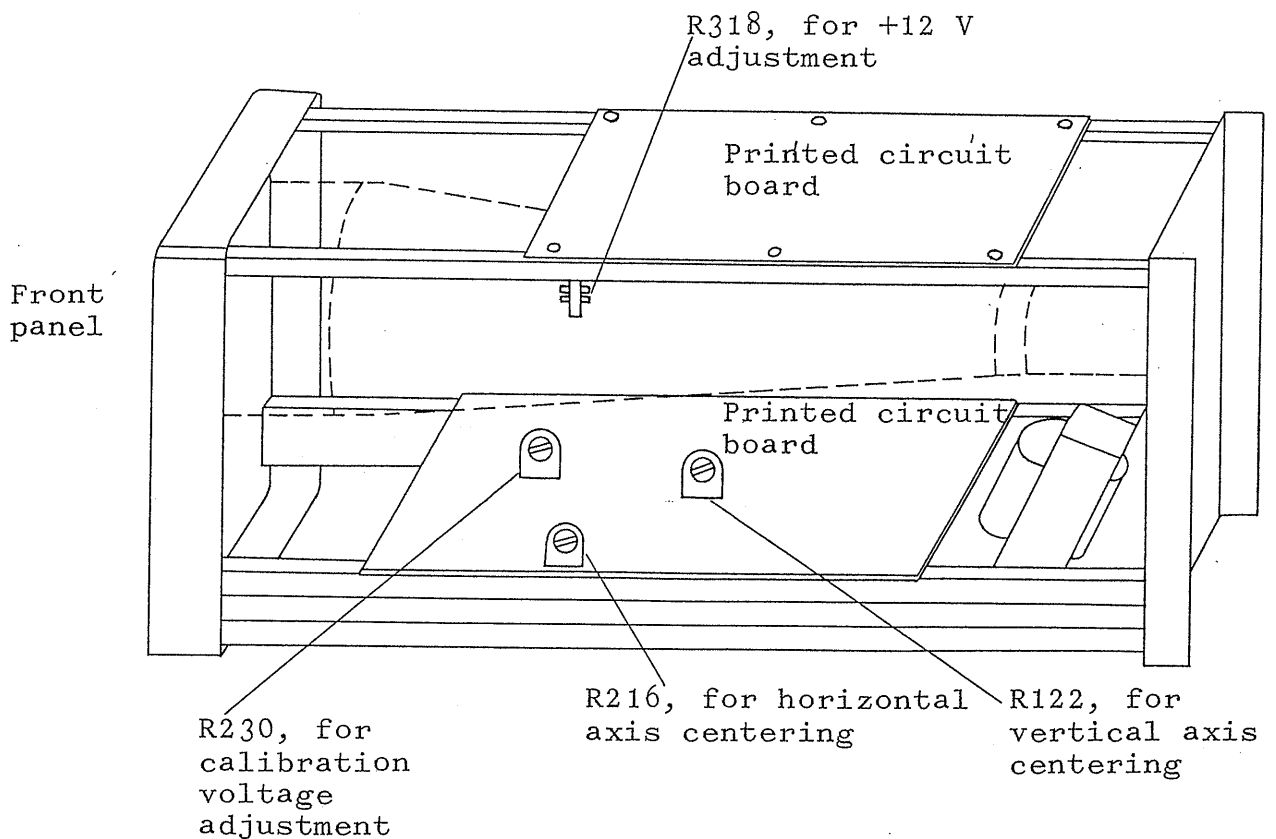

Adjustment of CAL mV_{p-p} (calibration voltage)

Adjustment of calibration voltage is seldom needed since the power source of the calibration voltage generator circuit is stabilized by using a reference diode. When adjustment should be necessary, adjust semi-fixed resistor R230 so that the voltage at the joint of R230 and R231 is $5 V_{p-p}$. For this voltage observation, an oscilloscope or p-p indication type voltmeter whose voltage sensitivity has been accurately calibrated should be connected to the joint of the above resistors.

Refer to the attached circuit diagram.

Adjustment of trace center

Semi-fixed variable resistors R122 and R216 are provided for centering the trace on the CRT screen, with the vertical and horizontal POSITION knobs set to the middle of their turning, range, respectively.

Without applying input signal, set both POSITION knobs to the middle of their turning range as illustrated below.

If the trace or spot on the CRT screen is off the center upward or downward, adjust it with R122; if rightward or leftward, with R216.

The above adjustment does not affect vertical and horizontal DC balance at all.

POSITION



The knob is in the middle of its turning range when the white dot or line on the knob is at the top.

For the locations of semi-fixed resistors R122 and R216, refer to the illustration under "Adjustment of power voltage," page 23.