



次の手順で機器にブラケットを取り付け、JIS 規格のラックに組み込みます。

1. 付属のねじを使用してブラケットを図のように取り付けます。付属のねじ（M4 x 10 皿ねじ）以外は使用しないでください。

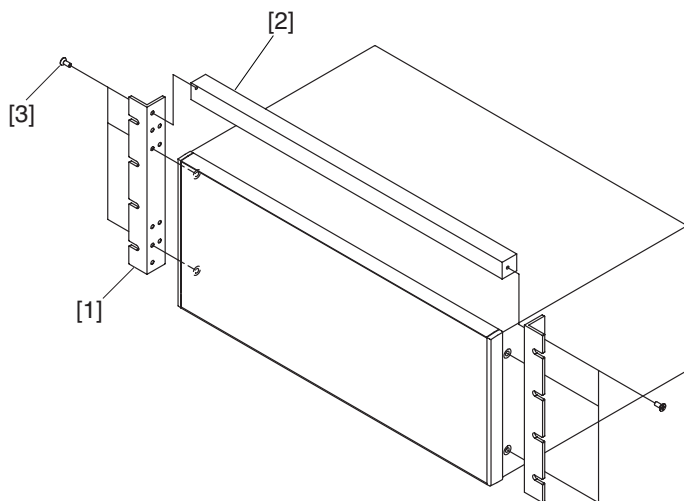


2. 付属のねじとワッシャを使用して JIS 規格のラックに取り付けます。

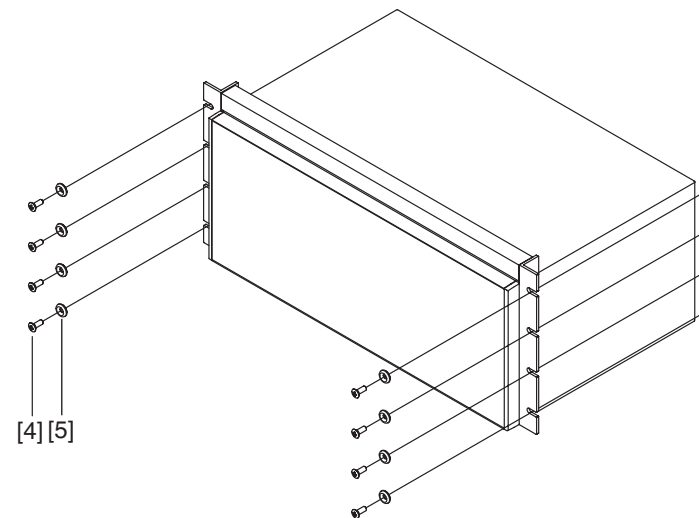

No.	品名	数量
1	Bracket KRB200	2
2	Bracket KRB200 top	1
3	Flat head screw M4 x 0.7 x 10	6
4	Oval head screw M5 x 0.8 x 14	8
5	Finishing washer 5CW	8



機器が落下する恐れがあります。
使用するラックに適合したサポートアングルを
取り付けて、本体を支持してください。



菊水電子工業株式会社

本社・技術センター 〒224-0023 横浜市都筑区東山田 1-1-3

TEL : 045-593-0200 (代)


<http://www.kikusui.co.jp/>

INSTRUCTION MANUAL


Bracket KRB200

Attach the mounting bracket to the instrument and install it to the JIS standard rack in the following procedure.

1. Attach the mounting bracket to the instrument using the provided screws as shown in figure. Do not use other than the provided screws (M4 x 10 flat-head screw).

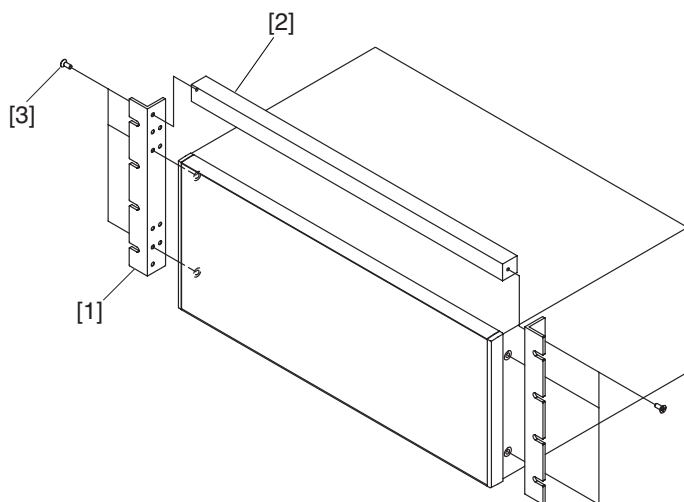


2. Install the rack mounting instrument to the JIS standard rack using the provided screws and washers.

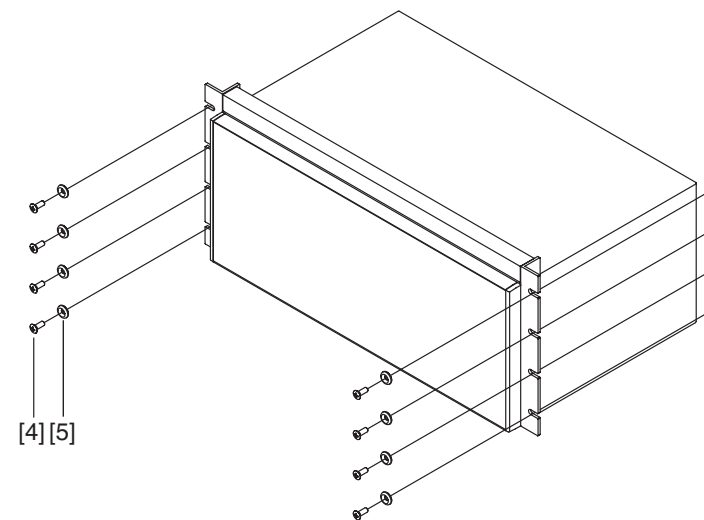

No.	DESCRIPTION	QTY
1	Bracket KRB200	2
2	Bracket KRB200 top	1
3	Flat-head screw M4 x 0.7 x 10	6
4	Oval head M5 x 0.8 x 14	8
5	Finishing washer 5CW	8



CAUTION The instrument may fall.
Install the suitable support angles
applying to the used rack system to
support the instrument.



KIKUSUI ELECTRONICS CORP.

1-1-3, Higashiyamata, Tsuzuki-ku, Yokohama, 224-0023, Japan

TEL : +81-45-593-7570 FAX: +81-45-593-7571

<http://www.kikusui.co.jp/>

Printed in Japan