

Operator's Manual

Portable Surface Resistivity/Resistance Meter

Model 272A



100 Housel Ave | PO Box 535 Lyndonville NY 14098
1-800-821-6001 | 585-765-2254 | fax: 585-765-9330 | monroe-electronics.com



WARRANTY

Monroe Electronics, Inc., warrants to the Owners, this instrument to be free from defects in material and workmanship for a period of two years after shipment from the factory. This warranty is applicable to the original purchaser only.

Liability under this warranty is limited to service, adjustment or replacement of defective parts (other than tubes, fuses or batteries) on any instrument or sub-assembly returned to the factory for this purpose, transportation prepaid.

This warranty does not apply to instruments or sub-assemblies subjected to abuse, abnormal operating conditions, or unauthorized repair or modification.

Since Monroe Electronics, Inc. has no control over conditions of use, no warranty is made or implied as to the suitability of our product for the customer's intended use.

THIS WARRANTY SET FORTH IN THIS ARTICLE IS EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES AND REPRESENTATIONS, EXPRESS, IMPLIED OR STATUTORY INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS. Except for obligations expressly undertaken by Monroe Electronics, in this Warranty, Owner hereby waives and releases all rights, claims and remedies with respect to any and all guarantees, express, implied, or statutory (including without limitation, the implied warranties of merchantability and fitness), and including but without being limited to any obligation of Monroe Electronics with respect to incidental or consequential damages, or damages for loss of use. No agreement or understanding varying or extending the warranty will be binding upon Monroe Electronics unless in writing signed by a duly authorized representative of Monroe Electronics.

In the event of a breach of the foregoing warranty, the liability of Monroe Electronics shall be limited to repairing or replacing the non-conforming goods and/or defective work, and in accordance with the foregoing, Monroe Electronics shall not be liable for any other damages, either direct or consequential.

RETURN POLICIES AND PROCEDURES

FACTORY REPAIR:

Return authorization is required for factory repair work. Material being returned to the factory for repair must have a *Return Material Authorization* number. To obtain an RMA number, call 585-765-2254 and ask for Customer Service.

Material returned to the factory for warranty repair must be accompanied by a copy of a dated invoice or bill of sale, which serves as a proof of purchase for the material.

Repairs will be returned promptly. Repairs are normally returned to the customer by UPS within ten working days after receipt by Monroe Electronics, Inc. Return (to the customer) UPS charges will be paid by Monroe Electronics on warranty work. Return (to the customer) UPS charges will be prepaid and added to invoice for out-of-warranty repair work.

EXPEDITED FACTORY REPAIR:

All material returned to the factory by air or by an overnight service will be expedited. Expedited factory repairs will be returned to the customer by the same mode of transportation by which the material was returned to the factory for repair (i.e., material returned to the factory by an overnight service will be returned to the customer by an overnight service).

NOTE: Return (to the customer) transportation expenses for expedited factory repairs will always be at the expense of the customer despite the warranty status of the equipment.

FACTORY REPAIRS TO MODIFIED EQUIPMENT:

Material returned to the factory for repair that has been modified will be not tested unless the nature and purpose of the modification is understood by us and does not render the equipment untestable at our repair facility. We will reserve the right to deny service to any modified equipment returned to the factory for repair regardless of the warranty status of the equipment.

INTRODUCTION:

The Monroe Electronics Model 272A Portable Surface Resistivity/Resistance Meter provides fast repeatable measurements of both surface resistivity and resistance to ground in one versatile instrument. Its improved accuracy and digital readout make it ideal for checking and evaluating static control products such as static dissipative bags, mats and work surfaces and resistance of work surfaces to ground. The Model 272A's convenient size, portability and rugged construction make this meter ideally suited for applications in a manufacturing environment.

FEATURES:

- Measures both surface resistivity and resistance to ground
- Easy to use - autozero - no adjustments required
- Portable - uses rechargeable battery for 8 hours continuous use
- Improved accuracy - ± 0.1 decade with digital readout
- Guarded ring electrode weighing 5 pounds conforms to standards
- Wide range of direct readings in ohms per square (Ω/\blacksquare) for surface resistivity or ohms (Ω) for resistance to ground
- Switch selectable measuring voltage - 10 volts or 100 volts
- Displays value in scientific notation or 3-place log

SPECIFICATIONS:

RANGE: From 8×10^3 to 2.0×10^{13} or 8×10^4 to $2.0 \times 10^{14} \Omega/\blacksquare$

INSTRUMENT ± 0.1 decade thru 10^{12} , ± 0.15 decade above 10^{12}

ACCURACY: (typical); ± 0.1 decade thru 10^9 , ± 0.15 decade thru 10^{11} ; ± 0.2 decade above 10^{12} (maximum)

MEASURING 10 volts for 8.0×10^3 to $2.0 \times 10^{12} \Omega$ or 8.0×10^4

VOLTAGE $2.0:10^{13} \Omega/\blacksquare$ and 100 volts for 1.1×10^5 to $2.0 \times 10^{13} \Omega$ or 1.1×10^6 to $2.0 \times 10^{14} \Omega/\blacksquare$

DISPLAY: 16x1 LCD alpha/numeric display will show:
Operation mode - Ω or Ω/\blacksquare
Readings in log or scientific notation
Applied voltage
Low battery
Also used in SETUP mode

POWER: Rechargeable battery with 100 VAC, 120 VAC or 230 VAC adapter/charger supplied. Power requirement is 16 VAC or DC (either polarity) @ 1.25A. Connector plug is 5mm OD; 2.55mm ID. Battery operation up to 8 hours continuous use

ELECTRODE: Guarded ring electrode recommended by ASTM D-257 weighing five pounds (2.7kg). The outer electrode is a ring having an inside diameter of 2.25 inches (5.72cm) and a width of 0.125 inches (0.32cm). The inner electrode is a disc with an outside diameter of 1.2 inches (3.05cm). The electrode assembly is separate from the meter and is connected to the meter by a cable 3 feet (91 cm) in length. A two-sided specimen support plate is included.

DIMENSIONS: Electrode - overall height - 4.0 inches (10.2cm) outside diameter - 3.0 inches (7.6cm) Meter - height - 2.5 inches (6.4cm) width - 6.0 inches (15.2cm) depth - 6.0 inches (15.2cm)

Recommended factory calibration cycle is one year.

HOW THE MODEL 272A WORKS:

Located on the insulating base of the electrode assembly are two concentric circular electrodes of conductive elastomeric material. The dimensions of these rings are such that when the assembly is placed on the flat surface of the material to be tested, ten squares of the material lie between the electrodes. When power is switched on a voltage is impressed on the outer ring and current flow in the interposed material is detected by the inner electrode thus defining the resistivity characteristics of the material. Internal circuitry of the Model 272A interprets this signal and provides a direct readout of the surface resistivity of the material under test in ohms per square. (Re. ASTM D-257, para. 3.5) In the resistance to ground mode, the test voltage is removed from the outer electrode and is applied to ground via a test lead supplied with the instrument. Current flowing between ground and the inner sensing electrode is detected and is converted to a direct readout of the resistance of the intervening path in ohms.

CAUTION DO NOT TOUCH ELECTRODES

1. Electrodes will become contaminated with skin oils.
2. When in operation, electrodes may be operating at a potential of 100 volts and are capable of delivering an annoying shock to the person touching them. Although the current capability is limited, a distinct hazard exists in the person's reaction to the shock.

BATTERY OPERATION:

Model 272A was designed to operate continuously for up to 8 hours on its internal battery when fully charged. A battery symbol will flash in the display when the battery needs recharging. To conserve battery power, the unit was shipped from the factory with its battery shutdown timer set for five minutes. This means that after five minutes of use (or non-use) the instrument will shut itself off. The timer is reset simply by pressing the ON-OFF switch. The default value may also be changed in software in the SETUP mode (described later). Optional default values are: 5 min., 10 min., 30 min. and NONE. Model 272A may also be line operated regardless of the state of its internal battery, although errors may be introduced by noise injected through the charging supply in this mode. To determine the degree of error, check readings in both modes. Battery operation will always produce the most reliable reading as long as the battery is charged.

During charging, the charge rate is reduced to a "float" rate as battery capacity is reached. The unit may be left on charge indefinitely. The battery is charged at a much lower rate when the unit is operating. The time-out feature is disabled while the charger is plugged in.

OPERATING ENVIRONMENT:

Proper operation of this instrument requires attention to its operating environment. Its sensitive circuitry is affected by uncontrolled static charges, ESD events and AC electric fields. Any of these may produce erroneous or erratic results. Generally, an ESD controlled environment is a preferred location for measurements.

PROGRAMMING:

Power-up default settings may be re-programmed in the SETUP MODE. Options are as shown below where the factory default is the first shown in the lists:

<u>OBJECTIVE</u>	<u>OPTION</u>
DISPLAY	SCI LOG
FUNCTION	Ω/\blacksquare OHMS
V SOURCE	10V 100V
AUTO OFF	5 MIN 10 MIN 30 MIN NONE
PROBE GAIN	* (see below)
RESET ALL	NO YES

To invoke the SETUP MODE, start with the instrument OFF. Press and hold the OHMS-OHMS/SQ push-button while switching power ON. The message "SETUP MODE" will be displayed very briefly and then the message "DISPLAY SCI" will appear. To alter the option, press the OHMS-OHMS/SQ push-button. To scroll the objectives, press the 10V-100V push-button. The PROBE GAIN options are 0.1 through 25.5 in increments of 0.1. Gain is factory preset to 10 for the probe which accompanies the Model 272A. PROBE GAIN SHOULD NOT BE CHANGED INDISCRIMINATELY IN THE FIELD.

Please note that the time-out feature is disabled in the setup mode and that if the battery voltage falls to a low value during programming, any newly selected options will be lost. At the RESET ALL objective, a NO response will accept any new power-up options and return to the operational mode using the new options. A YES response will reset any changes and return to the top of the list (DISPLAY SCI). A LOG display, the equivalent of the SCI display shown on Page 3 would be:

10.079 Ω/\blacksquare @10 V

where 10.079 is the common log value of the 12 gigaohm per square ($1.2E10 \Omega/\blacksquare$) input, not literally 10.079 ohms per square.

ERROR MESSAGES:

In addition to the flashing battery symbol that indicates the need for battery charging, any of several other error messages may appear on the screen:

MESSAGES

MEANING

ERROR MESSAGE 1:

VALUE TOO LOW

or *ERROR MESSAGE 2:*

VALUE TOO HIGH

Measured value beyond specified range of instrument, probe disconnected or incorrect measurement mode. If VALUE TOO HIGH is not displayed when probe is lifted in *CONFIDENCE CHECK*, check operating environment.

ERROR MESSAGE 3:

CANNOT AUTOZERO

Analog circuit malfunction or calibration problems.

ERROR MESSAGE 4:

PROBE SUPPLY LOW

Measuring voltage supply out of regulation due to overload or instrument failure.

MAINTENANCE TIPS:

The case of the Model 272A and the painted surfaces of its probe may be cleaned using a soft cloth saturated with a solution of warm water and a small amount of mild detergent and wrung out. Care should be taken not to get detergent solution inside of or on any part of the base of the probe. The contact electrodes should be cleaned whenever any accumulation of contaminants is noted as foreign materials on the faces may cause higher than normal indications. These parts should be cleaned by spraying or wiping gently with clean technical grade isopropyl alcohol.

RESISTANCE MEASUREMENTS:

Included with each Model 272A is a Model 96121-1 Surface-to-Ground Measuring Adapter. This adapter used with the probe and Model 272A meets requirements of the following standards for measurement of resistance to ground of flooring and work surface materials:

ASTM F-150

Standard Test Method for ELECTRICAL RESISTANCE OF CONDUCTIVE RESILIENT FLOORING

ESD ASSOCIATION STANDARD NO. 4.1

Worksurfaces - Resistive characterization

ESD ASSOCIATION STANDARD NO. 7.1

Floor Materials - Resistive characterization of materials

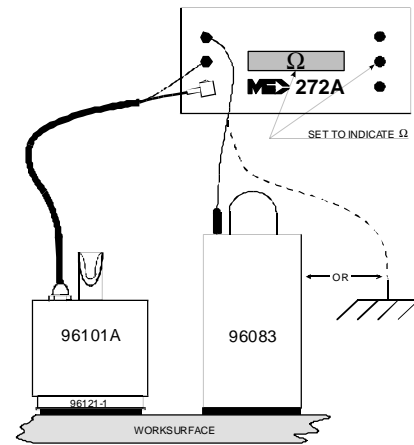


Figure 2
Setup for Surface-to-Ground and
Surface-to-Surface
Resistance Measurements

NOTE: The adapter serves as a protective cap for the probe during storage and must be removed to expose the concentric ring electrodes for resistivity measurements.

ASTM standards are available from:

American Society for Testing and Materials
1000 Barr Harbor Drive
West Conshohocken, PA 19428-2959
Phone (610) 832-9500
Fax (610) 832-9555

ESD Association standards are available from:

ESD Association, Inc.
7902 Turin Road
Suite 4
Rome, NY 13440-2069
Phone (315) 339-6937
Fax (315) 339-6793

Monroe Electronics, Inc. does not supply copies of standards.

To make a measurement of resistance from a surface to a ground point, connect the jack labeled "OHMS" to the ground point, set the electrode on the surface and switch to the "OHMS" mode (see Figure 2).

Surface-to-surface measurements, also directed in these standards, require the use of a second electrode (Monroe Electronics Model 96083) as shown in Figure 2. Model 96083 electrodes are included in Models 96085-1 and 96085-2 electrode sets or they may be ordered separately.

APPLICATION NOTE APNE-0002

PRACTICAL VOLUME RESISTIVITY MEASUREMENTS with Monroe Model 272A

Included with Model 272A is a P/N 96117-1/22A specimen support plate. This support plate provides a durable finish on the insulated side and also provides a smooth metallic surface on the opposite side for volume resistivity or bulk resistance measurements of materials.

The combination of this plate, the P/N 96101A-1 probe and the Model 272A instrument meets the guidelines set forth in ASTM D-257 and IEC 93 Standards for guarded-ring testing of volume resistivity of solid, homogeneous electrical insulating materials, generally in sheet form. Connections for guarded measurements are shown in Figures 3 and 4.

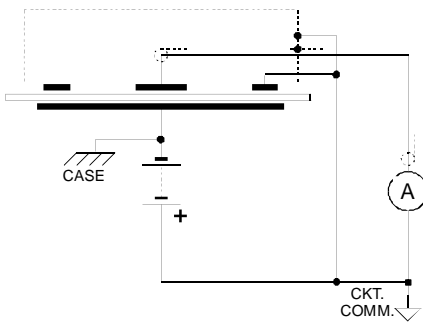


Figure 3: Setup for Guarded Measurement of Volume Resistivity

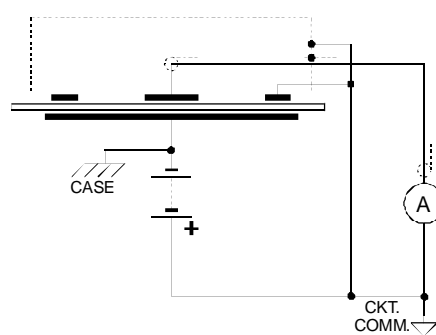


Figure 4: Schematic Representation

Volume resistivity, ρ_v , must always be calculated because the thickness of the test specimen is one of the measurement variables. The ASTM D-257 (or IEC 93) formula for ρ_v is:

$$\mathbf{r}_v = \frac{A}{t} R_m \text{ ohm} \cdot \text{cm}$$

where: A = Effective area of measuring electrode in cm^2

t = Thickness of test specimen in cm

R_m = Measured resistance in ohms

For the 96101A-1 probe the effective area of the measuring electrode is 7.3 cm^2 thus:

$$\mathbf{r}_v = \frac{7.3}{t} R_m \text{ ohm} \cdot \text{cm}$$

Appendix X2 in the ASTM standard further addresses the modification of the effective area of the measuring electrode in the guarded ring configuration.

The Connections for unguarded measurements are given in Figure 5. Factors for converting meter readings (in Ω) directly to volume resistivity (unit $\Omega.cm$) are presented in Table 1. Above information is presented as an overview of some of the complications involved in the use of the concentric or guarded ring type electrode. Either of the standards should be consulted for further details.

SIMPLIFIED METHOD

Most materials commonly being tested in today's world of ESD awareness are intended not to be electrically insulative. For specimens that have negligible surface leakage, an unguarded measurement based on the actual area of the (1.2" dia.) center electrode greatly simplifies the calculations. For material samples less than 0.060" thick, the errors introduced into an unguarded measurement are usually small enough to be negligible.

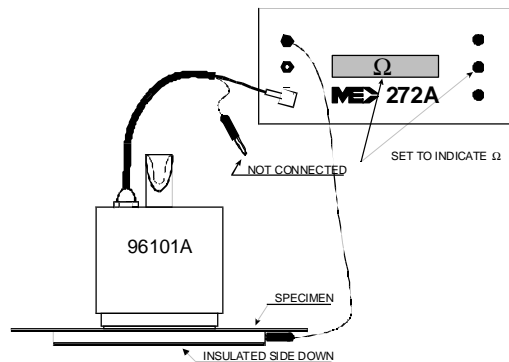


Figure 5
Connections for Un-guarded Measurement of
Volume Resistivity

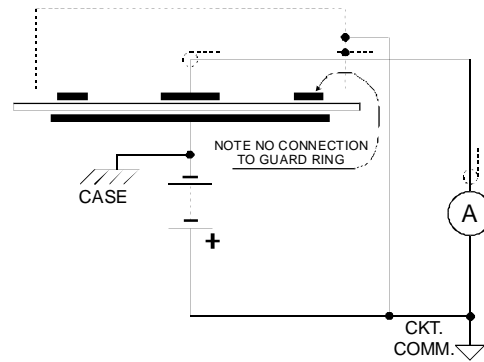


Figure 6:
Schematic Representation

Material Thickness	Factor	Material Thickness	Factor
0.005" (0.13mm)	575	0.035" (0.89mm)	82
0.010" (0.25mm)	287	0.040" (1.02mm)	72
0.015" (0.38mm)	192	0.045" (1.14mm)	64
0.020" (0.51mm)	144	0.050" (1.27mm)	57
0.025" (0.64mm)	115	0.055" (1.40mm)	52
0.030" (0.76mm)	96	0.060" (1.52mm)	48

Table 1

TO USE THIS TABLE-

- 1) Arrange test setup as in Figure 5.
- 2) Set Model 272A to "ON".
- 3) Select "OHMS". The " Ω " symbol will appear in the display.
- 4) Select measuring voltage (10V or 100V).
- 5) Record the reading and the material thickness.
- 6) Multiply the reading by the factor given in the table for the value of volume resistivity in $\Omega.cm$.