



**ROHDE & SCHWARZ**

Test and Measurement  
Division

## **Release Notes**

# **R&S FSQ-K70**

## **Vector Signal Analysis Application Firmware**

### **Release 4.60**

for R&S FSU, FSQ, FSG, FMU, FSUP  
Analyzer Firmware 4.6x

#### **New Features:**

- **New user filter set "HALF SINE" supporting ZigBee (IEEE 802.15.4)**
- **New modulation type  $\pi/8$ -D8PSK**
- **Additional Symbol Mapping files for TETRA and APCO-25 Phase 2**

**Release Note Revision: 4**

Printed in the Federal  
Republic of Germany

## Contents

<b>History .....</b>	<b>3</b>
<b>General Topics .....</b>	<b>3</b>
Hardware Requirements .....	3
Compatibility of the R&S FSQ-K70 Vector Analysis Application Firmware with other Firmware Releases .....	4
Firmware Update of the R&S FSQ-K70 Vector Analysis Application Firmware .....	5
Enabling the Application Firmware via License Key Code Entry .....	6
<b>New Functions in Version 4.60 .....</b>	<b>6</b>
<b>Improvements with Version 4.60.....</b>	<b>6</b>
<b>Known Issues with option R&amp;S FSQ-K70 Vector Analysis.....</b>	<b>7</b>
<b>Modified Functions.....</b>	<b>7</b>
<b>Modifications to the Operating Manual and Supplements .....</b>	<b>8</b>
Last minute changes to the operating manual.....	9
Menu Overview - Softkeys .....	9
Setting Parameters – MODULATION SETTINGS Softkey.....	9
Menu TRACE - NEXT .....	10
Glossary and Formulae .....	14
Trace-based Evaluations .....	14
Summary - Evaluations.....	14
Remote Control Commands .....	16
DISPlay subsystem.....	16
FORMat subsystem .....	17
MMEMory subsystem .....	18
SENSe subsystem.....	19
Remote Control Commands - Programming Examples .....	21
Performing a Measurement with OPC Synchronization .....	21
Creating a Search Pattern .....	21

<b>Customer Support.....</b>	<b>23</b>
Technical support – where and when you need it .....	23
Up-to-date information and upgrades .....	23

## History

Date	Rel Note Rev	Changes
20 June 2010	1	First revision for Vector Analysis Application Firmware 4.60.
12 October 2010	2	New hot line phone number for calls from Europe.
07 March 2011	3	New chapter "Customer Support".
06 June 2011	4	Entry for FSUP.

## General Topics

### Hardware Requirements

The option R&S FSQ-K70 requires certain minimum board revisions of the Wideband Detector Board.

For R&S FSUP at least model 08 of Wideband Detector Board is required for R&S FSQ-K70:

This can be checked in the SPECTRUM -> SETUP -> SYSTEM INFO menu with softkey HARDWARE INFO. For component WBDET with order number 1130.3086 is required at least:

Model	Revision	Sub Revision	
			for
3	4	$\geq 8$	R&S FSQ (with CPU-Board 1091.2520) <b>or</b>
3	$\geq 5$		R&S FSQ (with CPU-Board 1091.2520) <b>or</b>
5			R&S FSQ (with CPU-Board 1091.2520), R&S FSU (with CPU-Board 1091.2520) <b>or</b>
8			R&S FSU (with CPU-Board 1091.3104), R&S FSQ (with CPU-Board 1091.3104), R&S FSUP, R&S FSG, R&S FMU

## Compatibility of the R&S FSQ-K70 Vector Analysis Application Firmware with other Firmware Releases

The following table shows the compatible versions of the basic analyzer firmware and the Vector Analysis Application Firmware:

**Table of compatible versions:**

R&S FSQ-K70 Application Firmware	R&S FSU Basic Firmware	R&S FSQ Basic Firmware	R&S FSMR Basic Firmware	R&S FSUP Basic Firmware	R&S FMU Basic Firmware	R&S FSG Basic Firmware
4.60	4.61	4.65	-	Please refer to the FSUP release notes	-	4.69
4.50 SP3	4.51 SP1	4.55 SP2	-		-	4.59 SP1
4.50 SP2	4.51	-	-		-	-
4.50 SP1	-	4.55 SP1	-		-	4.59
4.50	-	-	-		-	4.59
4.40 SP1	-	-	-		-	-
4.40	4.41	4.45	-		-	4.49
4.30 SP1	4.31 SP1	4.35 SP1	4.36		4.38	4.39 SP2
4.30	4.31	4.35	-		-	4.39
4.20 SP2	4.21 SP1	4.25 SP1	4.26		-	4.29 SP3
4.20 SP1	4.21	4.25	-		-	4.29
4.20	4.21	4.25	-		-	4.29
4.10	4.11	4.15	4.16		-	-
4.01	-	-	-		4.08	-
4.00 SP2	4.01 SP3	4.05 SP3	-		-	-
4.00 SP1	-	-	4.06		-	-
4.00	4.01	4.05	-		-	-
3.90 SP1	-	3.95 SP2	-		-	-
3.90	-	3.95	3.96		-	-
3.80	-	3.85				
3.70	-	3.75	-		-	-
3.60	-	3.65	-		-	-
3.50 SP1	-	3.55 SP2	-		-	-
3.50	-	3.55	-		-	-
3.40	-	3.45	-		-	-
3.30	-	3.35	-		-	-
3.28	-	3.25	-		-	-
3.24	-	3.15	-		-	-
3.21	-	3.05 SP1	-		-	-
3.20	-	3.05	-		-	-

R&S FSQ-K70 Application Firmware	R&S FSU Basic Firmware	R&S FSQ Basic Firmware	R&S FSMR Basic Firmware	R&S FSUP Basic Firmware	R&S FMU Basic Firmware	R&S FSG Basic Firmware
2.30	-	2.35	-		-	-
2.28	-	2.25	-		-	-
2.24	-	2.15	-		-	-
1.21	-	2.05	-		-	-
1.00	-	1.85	-		-	-
-	-	1.65	-		-	-
-	-	1.55	-		-	-

The FSQ-K70 application firmware versions 3.xx or 4.xx requires Windows XP. For NT based instruments a Windows-XP upgrade kit FSQ-U2, order # 1162.9696.02 is available.

**Note:**

*Applications with version number 3.xx or 4.xx are only compatible with basic firmware 3.yy or 4.yy (see table above). Do not install them on basic firmware versions below 3.00!*

## Firmware Update of the R&S FSQ-K70 Vector Analysis Application Firmware

Since basic firmware version 4.2x a ZIP file with the update sets of the basic system firmware and all available applications is provided. This ZIP file is available in the instruments FIRMWARE section, e.g. R&S FSU of the Service Board on GLORIS.

Please follow the steps described in the instrument's basic firmware release note to perform a complete firmware update.

## Enabling the Application Firmware via License Key Code Entry

This section can be skipped if the option key was entered once.

After installing the application firmware package a license key for validation must be entered. The license key is printed either on a label on the rear panel of the R&S FSQ or delivered as a part of the R&S FS-K70 Vector Analysis Application Firmware package.

The key sequence for entering the license key is:

SETUP - GENERAL SETUP – OPTIONS - INSTALL OPTION

Use the numeric keypad to input the license key number and press ENTER.

- On a successful validation the message 'option key valid' will appear.
- If the validation failed, the application firmware is not installed.  
The most probable reason will be that the instrument is not equipped with the correct basic firmware version. Therefore a message box will appear asking for installation of the correct basic firmware version.  
If the application firmware package was not installed prior to entering the license key code, a message will appear asking for installation of the application firmware package.  
**In any case please make sure that the correct basic firmware version and the application firmware package is installed prior to entering the license key code.**

## New Functions in Version 4.60

- New user filter set "HALF SINE" supporting ZigBee (IEEE 802.15.4)
- New modulation type  $\pi/8$ -D8PSK
- Additional Symbol Mappings available for TETRA and APCO-25 Phase 2

## Improvements with Version 4.60

The version numbers in brackets indicate the version in which the issue was observed for the first time.

**1. (V4.50SP2) The first Marker Peak Search sometimes fails after the number of symbols or points per Symbol has been changed.**

**2. (V4.50SP2) The application is not able to save an equalizer filter in manual operation.**

The application may crash or create a file ".vae". The user specified file name is ignored. In remote operation the save operation is performed without any problem.

**3. (V4.50SP2) Demod Next Right fails to find next pattern in Multi Mode.**

Function Demod Next Right fails to find the next pattern in multi mode using the following settings:

- MULTI ZOOM ON
- BURST SEARCH ON with MEAS ONLY ON BURST active
- PATTERN SEARCH ON with MEAS ONLY ON PATTERN active
- Perform an I/Q data capture by starting a single sweep.
- Use softkey DEMOD NEXT RIGHT to search the next pattern.

The search function sometimes skips one of the bursts even though the correct search pattern is part of the burst.

**4. (V4.50SP2) The modulation & Mapping dialog does not mark the current selection.**

## Known Issues with option R&S FSQ-K70 Vector Analysis

The version numbers in brackets indicate the version in which the error was observed for the first time.

**1. (V4.50) Selection of User QAM Mapping files does not work in remote operation.**

Work around: Define a new generic standard using this demodulation and mapping in manual operation and select this generic standard in remote operation.

## Modified Functions

The behaviour of the following functions changed compared to earlier versions [the number in brackets indicates the firmware version that introduced the individual change]:

1. (V3.60) **EXPORT STANDARD: Query before overwriting existing file in manual operation.**
2. (V3.60) **Menu HOME VSA - FACTORY DEFAULTS now support PATTERNS, too.**
3. (V3.60) **Expanded range for Symbol Rate. The lower limit is now 100 Hz.**
4. (V3.60) **A trace in VIEW state in analyzer mode is set to CLR/WRITE when leaving the vector analysis mode.**
5. (V3.80) **Expanded range for FSK Ref. Deviation. The upper limit is now 1.5 \* Symbol Rate.**
6. (V3.80) **Measurements at low frequencies using baseband inputs of option FSQ-B71 by a digital down conversion are now supported.**
7. (V3.80) **Absolute marker position for marker 1 added for measurement result AM/AM - AM/PM conversion.**
8. (V3.80) **SAVE AS STANDARD additionally stores statistics parameter settings (X-AXIS QUANTIZE, X-axis and Y-axis scaling).**
9. (V3.80) **Default focus for NEW PATTERN dialog is change to pattern name.**
10. (V3.90) **Support of option FSQ-B100: Extended Record Length.**
11. (V4.00) **External trigger level in steps 0.1V over the complete range of 0.5V to 3.5V.**
12. (V4.20) **Support for instrument R&S FSG.**

**13. (V4.20) Result SYMBOLS & MOD ACC: Calculation of SNR (signal-to-noise ratio) changed.**

Before version 4.20, the SNR calculation is dependent on the EVM CALC setting (MAX SYMBOL / SIGNAL MEAN POWER). Since version 4.20 the SNR value is only referenced to the mean power. EVM CALC setting is ignored for SNR calculation.

**14. (V4.20) Trace Export of I/Q Data (RAW DATA) in WAVEFORM format.****15. (V4.30) Softkeys Signal Source Type (I+j\*Q, I Only, Q Only) are only available if baseband input is selected.****16. (V4.30) Multi Mode: Changing the Zoom Start window has no effect.**

The Capture Buffer Trace is not updated according to the new zoom window position, if the zoom start position is changed at the current zoom window is located at the end of the I/Q capture buffer.

**17. (V4.30) Statistics measurement: New function field indicates voltage/level interval.**

The interval used for the statistics evaluation is indicated with a new function field at the left top corner of the grid replacing the reference level indication.

**18. (V4.30) New windows dialogs available for File Import/Export functions.**

New dialog with browser functions are now available to export traces or configure the import / export path for Standards, Pattern, Filters, Equalizers.

**19. (V4.40) Export and Import of I/Q RAW data.****20. (V4.50) Extended maximum FSK Reference Deviation (8 \* Symbol Rate).****21. (V4.50) Additional Trace ASCII Export information (Preamplifier, Transducer).****22. (V4.50) Direct Ex-IQ-Box Configuration Dialog access.****23. (V4.50) New sub menus for signal path dependent softkeys with option R&S FSQ-B71 (Analog Baseband Input) and R&S FSQ-B17 (Digital baseband Input).****24. (V4.60) New filter set "HALF SINE" supporting ZigBee (IEEE 802.15.4).****25. (V4.60) New modulation type  $\pi/8$ -D8PSK.****26. (V4.60) Additional Symbol Mappings available for TETRA and APCO-25 Phase 2.**

For $\pi/4$ -DQPSK:	"APCO25 Phase 2"
$\pi/8$ -D8PSK:	"APCO25 Phase 2"
	"TETRA"

## Modifications to the Operating Manual and Supplements

The R&S FSQ-K70 analyzer functions are included in a separate new manual set. Please refer to the following order numbers:


- 1161.8073.42-12 (English)
- 1161.8073.41-12 (German)

The corresponding PDF-Files are separately available on the service board.



## Last minute changes to the operating manual

### Menu Overview - Softkeys

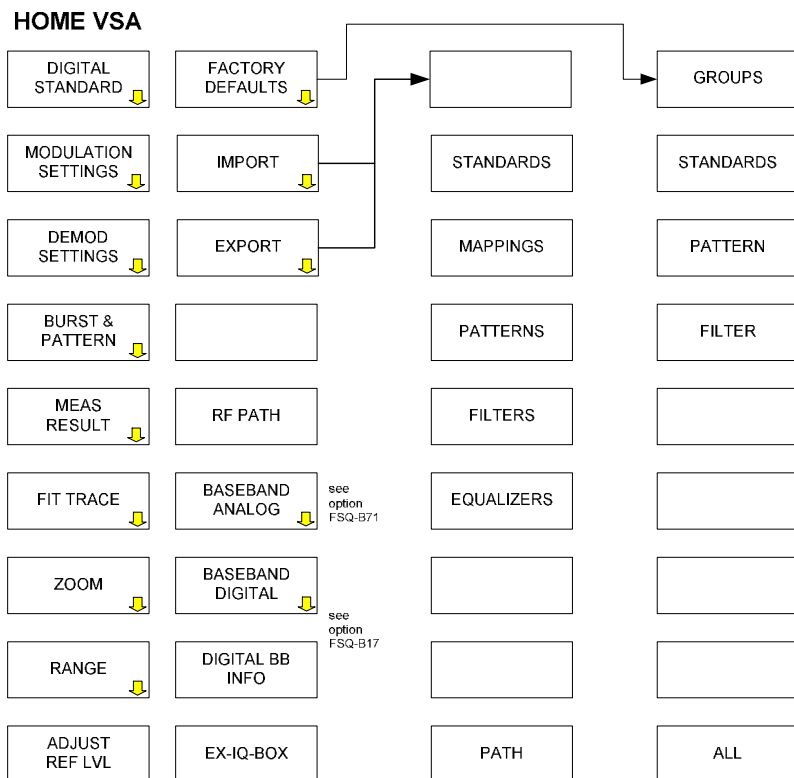

### Setting Parameters – MODULATION SETTINGS Softkey

#### MODULATION FILTER

MODULATION FILTER SET			
TRANSMIT FILTER	RECEIVE FILTER	MEAS FILTER	SET
RC	NONE	NONE	RC
RRC	RRC	RRC	RRC
GAUSS	NONE	NONE	GAUSS
GAUSS_LINEARIZED	EDGE_ISI	EDGE_MEAS	EDGE
CDMA2K_1X_FWD_TX	CDMA2K_1X_FWD_ISI	CDMA2K_1X_FWD_ISI	CDMA2K 1F
CDMA2K_1X_REV_TX	CDMA2K_1X_REV_ISI	CDMA2K_1X_REV_ISI	CDMA2K 1R
APC025_C4FM_TX	APC025_C4FM_ISI	APC025_C4FM_ISI	APC025C4FM
APC025_F4FM_TX	APC025_F4FM_ISI	APC025_F4FM_ISI	APC025F4FM
HALF_SINE	NONE	NONE	HALF SINE

**Fig. 152 Filter selection list**

As of firmware version 4.60 an additional user filter set "HALF SINE" is available. This filter set is required for ZigBee (IEEE 802.15.4) measurements.

For details please refer to application note "1EF55: EVM Measurements for ZigBee signals in the 2.4 GHz band" available on the R&S download area.

## Menu TRACE - NEXT

TRACE	SELECT TRACE	MIN HOLD	The <i>TRACE</i> key opens a menu for setting the trace functions.
	CLEAR / WRITE	AVG MODE (LOG)	<i>SELECT TRACE</i> selects the trace of the active measurement screen.
	MAX HOLD	FILE EXPORT	The trace <b>display mode</b> can be selected as follows:
	AVERAGE	FILE IMPORT	<i>CLEAR WRITE</i> Overwrite mode; the old trace is deleted after each measurement and overwritten by the new trace.
	VIEW	DATA TRACE	<i>VIEW</i> The current trace is frozen.
	BLANK	DATA RAW	<i>BLANK</i> The selected trace is blanked.
	SWEEP COUNT	HEADER ON OFF	<b>Weighting</b> of the complete trace is selected as follows:
	RMS	DECIM SEP . ,	<i>AVERAGE</i> The average value is determined.
			<i>MAX HOLD</i> The maximum value is determined.
			<i>MIN HOLD</i> The minimum value is determined.
			<i>RMS</i> The calculation of the RMS value is determined.

**Export** of all active traces is selected as follows:

*FILE EXPORT* All active traces are stored  
*DATA RAW* The data type RAW DATA is selected. The formats ASCII and WAVEFORM are supported.  
**Note:** Files saved with format WAVEFORM are loadable by R&S SMU signal generator.

*HEADER* A file header is created or not  
*DECIM SEP* The decimal separator is selected.

*FILE IMPORT* Imports the I/Q RAW data previously stored with FILE EXPORT (DATA RAW, format binary).

**Export** of all active traces is selected as follows:

*FILE EXPORT*

All active traces are stored.

**Remote command:**

MMEM:STOR:TRAC 1, 'D:\rawdat'

*DATA RAW*

The data type RAW DATA is selected. The formats ASCII, WAVEFORM and BINARY are supported.

ASCII Exports the selected data (TRACE / RAW) in ASCII file format.

WAVEFORM Files saved with format are loadable by R&S SMU signal generator R&S SMU signal generator.

BINARY Exports the I/Q RAW data and the VSA user parameter settings in a binary format. The VSA settings are stored in <file\_name>.VAV, the RAW data are stored in <file\_name>.BIN. Files saved with this format are loadable by function FILE IMPORT.

**Note:** The required disk space to store the I/Q RAW data depends on the specified RECORD LENGTH and might exceed the available disk space.

**Remote command:**

FORMat:DEXPort:RAW:FORMat ASCii | BINary | WAVeform'

*HEADER*

A file header is created or not

*DECIM SEP*

The decimal separator is selected.

**Trace Export:**

Since version 4.50 the additional lines "Preamplifier" and "Transducer" are added to the export file.

**Example:**

	Content of file	Description
File header	Type;FSQ;	Instrument model
	Version;4.55;	Firmware version
	Date;08.Jun 2009;	Date record storage date
	Mode;VSA;DB1.50	Instrument operating mode
	Digital Standard;GSM_NB;	Digital standard
	Demodulator;DMSK;	Demodulation
	Center Freq;100000000;Hz	Center frequency
	Freq Offset;0;Hz	Frequency offset
	Ref. Level;-20;dBm	Reference level
	Level Offset;0;dB	Level offset
	RF Att;5;dB	Input attenuation
	El Att;0;dB	Input attenuation (with option FSU-B25 only)
	Symbol Rate;270833;Hz	Symbol rate
	Transmit Filter;GAUSS;	Filter settings
	Receive Filter;NONE;	
	Measurement Filter;NONE;	
	Raw Data Filter;ON;	
	Alpha BT;0.300000;	Signal source
	Signal;RF Input;	
	Result Length;160;	
	Record Length;1500;	
	Points per symbol;4;	Points per symbol
	x Axis Start;-9.000000;symbols	Scaling of x-axis
	x Axis Stop;150.750000;symbols	
	y per div;1.000000;deg	Scaling of y-axis
	Ref Value y-Axis;0.000000;deg	
	Ref Value Position;50.000000;%	
	Sweep Count;0;	Number of sweeps set
	Preamplifier;OFF;	Preamplifier state (OFF, if no preamplifier is available)
	Transducer;OFF;	Transducer state (always OFF)

<b>Data part of the file</b>	Trace;1;	Trace
<b>Trace 1 / Screen A</b>	Screen;A;	Screen A
	Meas Result;Error;	Measurement:
	Meas Signal;Phase;	Error Signal, Phase Error
	Demodulator;DMSK;	
	ResultMode;Trace;	Trace mode
	x Unit;symbols;	Unit of x and y values
	y Unit;deg;	
	Trace Mode;CLR/WRITE;	Display mode of trace: CLR/WRITE, AVERAGE, MAXHOLD, MINHOLD
	Values;640;	Number of measurement points
	1.834240	Measured values::
	1.662848	<real>, <imag>
	.....	<imag> being available only with Real/Imag, Polar- and
	-0.127578	Constellation diagrams.
	-0.889226	
<b>Data part of the file</b>	Trace;1;	Trace
<b>Trace 1 / Screen B</b>	Screen;B;	Screen B
	Meas Result;Meas;	Measurement:
	Meas Signal;Magnitude;	Meas Signal, Magnitude
	Demodulator;DMSK;	
	ResultMode;Trace;	
	x Unit;symbols;	
	y Unit;deg;	
	Trace Mode;CLR/WRITE;	
	Values;640;	
	0.681856	
	0.680534	
	....	
	0.682217	

## Glossary and Formulae

### Trace-based Evaluations

Test parameter	Formula
Error Vector Magnitude = EVM	$EVM(t) = \frac{ EV(t) }{C}$ ; In case of Offset-QPSK please observe the influence of the softkey "Offset EVM ON/OFF" on nominator and denominator.

### Summary - Evaluations

SNR ( MER) (Signal-to-noise ratio)	$SNR = 10 \log_{10} \left( \frac{\text{signal power}}{\text{noise power}} \right) = \frac{\frac{1}{N} \sum_{n=0}^{N-1}  REF(n \cdot T_{symbol}) ^2}{\frac{1}{N} \sum_{n=0}^{N-1}  MEAS(n \cdot T_{symbol}) - REF(n \cdot T_{symbol}) ^2}$ <p>The <b>SNR</b> (signal-to-noise ratio) is the quotient of the <b>signal power</b> of the ideal signal (REF signal) and the <b>noise power</b>. The signal power is calculated as the mean power of the ideal signal (REF signal) at symbol decision points. The noise power is calculated as the mean power of the error signal, i.e. the difference of the measured signal and the corresponding ideal signal (MEAS-REF signal), at symbol decision points. For VSB, only the power of the real part is considered.</p> <p>The definition of the SNR has been changed with firmware version 4.20. In older versions the SNR was calculated in the same way as the EVM and did depend on the softkey "EVM CALC".</p> <p>The parameter "EVM calc" does always influence the calculation of EVM.</p>
Normalization constant C (not VSB)	$C = \sqrt{\frac{1}{K} \sum_k  REF(k) ^2} = \text{sqrt( mean power of the symbol decision instants)}$ <p>But if the softkey "EVM CALC" is set to "MAX SYMBOL POWER", the factor C is not calculated as given above, but set to the constant ideal value of the maximum symbol magnitude.</p> <p>In case of Offset-QPSK please observe the additional influence of the softkey "OFFSET EVM ON/OFF" on the determination of the symbol instants in the I- and Q-part of the REF signal.</p>

Normalization constant C (VSB only)	$C = \sqrt{\frac{1}{K} \sum_K  \text{Re}\{REF(k)\} ^2} = \text{sqrt}(\text{mean power of the symbol decision instants}).$ <p>But if the softkey "EVM CALC" is set to "MAX SYMBOL POWER", the factor C is not calculated as given above, but set to the constant ideal value of the maximum symbol magnitude.</p>
RMS_EVM (not VSB)	$RMS\_EVM = \sqrt{\frac{1}{K} \sum EVM(k)^2}$ <p>In case of Offset-QPSK please observe the influence of the softkey "Offset EVM" on the EVM trace.</p>
RMS_EVM (VSB only)	$RMS\_EVM = \sqrt{\frac{1}{K} \sum \text{Re}\{EVM(k)\}^2}$
Origin_Offset (logarithmic measure for IQ_Offset)	$OriginOffset = 10 \log_{10} \left( \frac{ IQ\_Offset ^2}{C^2} \right)$ <p>Note: For the normalization of the "Origin Offset" the denominator C does not depend on the softkey "EVM CALC" and "OFFSET EVM". The calculation assumes that they are set to "MEAN SIGNAL POWER" respectively "OFFSET EVM OFF".</p>

## Remote Control Commands

### DISPlay subsystem

**DISPlay[:WINDow<1|2>]:TRACe<1 to 3>:MODE** WRITe | VIEW | AVERAge | MAXHold | MINHold | RMS

This command defines the type of display and the evaluation of the traces in the selected measurement window. WRITE corresponds to the Ctr/Write mode of manual operation. The trace is switched off (= BLANK in manual operation) with the DISPlay[:WINDow<1|2>]:TRACe<1 to 3>[:STATe] command. The number of measurements for AVERAge, RMS, MAXHold and MINHold is defined with the [SENSe<1|2>:]AVERAge:COUNT or [SENSe<1|2>:]SWEep:COUNT command. Synchronization to the end of the indicated number of measurements is only possible in single-sweep mode.

**Parameter:**

- WRITe: Activates the overwrite mode for the collected measured values, i.e. the trace is overwritten by each sweep.
- MAXHold: Saves for each sweep the maximum of the previously stored/currently measured values in the trace memory.
- MINHold: Saves for each sweep the smallest of the previously stored/currently measured values in the trace memory.
- AVERAge: Activates the linear averaging function. The average is formed over several sweeps.
- RMS: Activates the root square averaging function. The average is formed over several sweeps.

**Example:**

```
*RST"
":INST:SEL DDEM"           ' enter VSA option
                             ' configure Screen A result:
":CALC1:FEED 'XTIM:DDEM:ERR:MPH'" ' select error signal
":CALC1:FORMat PHAS"        ' select format phase
":DISP:WIND1:TRAC:MODE RMS" ' select RMS Averaging
```

**Characteristics:**

- \*RST value: WRIT
- SCPI: device-specific

**DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALE]:PDIVision** <numeric\_value>

This command defines the scaling of the y-axis in the current unit. The default value depends on the selected measurement result and format (e.g. Meas Signal – Magnitude).

The numeric suffix under TRACe<1...3> is irrelevant.

**Example:**

```
*RST"
":INST:SEL DDEM"           ' enter VSA option
":CALC1:FEED 'XTIM:DDEM:MEAS'" ' select meas signal
                             ' select format phase
":CALC1:FORMat PHAS"
":DISP1:TRAC:Y:PDIV 10.0"  ' sets y-axis /div to 10 deg
```

**Characteristics:**

- \*RST value: --
- SCPI: device-specific



**DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]: RPOStion 0...100PCT**

This command defines the position of the reference value for the y-axis. The default value depends on the selected measurement result and format (e.g. Meas Signal – Magnitude at 100%, Meas Signal – Phase at 50%).

The numeric suffix under TRACe<1...3> is irrelevant.

**Example:**

```
*RST"
":INST:SEL DDEM"
":CALC1:FEED 'XTIM:DDEM:MEAS'"
":CALC1:FORMat PHAS"
":DISP1:TRAC:Y:PDIV 10.0"
":DISP1:TRAC:Y:RPOS 50.0"
```

' enter VSA option  
' select meas signal  
' select format phase  
' sets y-axis /div to 10 deg  
' ref value position at 50%

**Characteristics:** \*RST value: --  
SCPI: device-specific

**DISPlay[:WINDow<1|2>]:TRACe<1...3>:Y[:SCALe]:RVALue <numeric\_value>**

This command defines the reference value for the y-axis of the measurement diagram.

The numeric suffix under TRACe<1...3> is irrelevant.

**Example:**

```
*RST"
":INST:SEL DDEM"
":CALC1:FEED 'XTIM:DDEM:MEAS'"
":CALC1:FORMat PHAS"
":DISP1:TRAC:Y:PDIV 10.0"
":DISP1:TRAC:Y:RPOS 50.0"
":DISP1:TRAC:Y:RVAL 20.0"
```

' enter VSA option  
' select meas signal  
' select format phase  
' sets y-axis /div to 10 deg  
' ref value position at 50%  
' sets ref value to 20 deg

**Characteristics:** \*RST value: --  
SCPI: device-specific

**FORMat subsystem****FORMat:DEXPort:RAW:FORMat ASCii | WAVeform | BINary**

This command defines the output format of the RAW data file export function.

**Parameter:** ASCii ASCII file format  
WAVeform Format WAV can be read e.g. by signal generator R&S SMU.  
BINary Exports the I/Q RAW data and the VSA user parameter settings in a binary format. Files saved with this format are loadable by function MMEM:LOAD:TRAC.  
Note: The required harddisk space to store the I/Q RAW data depends on the RECORD LENGTH specified.

**Example:**

```
:FORM:DEXP:MODE RAW"
:FORM:DEXP:RAW:FORM WAV"
:MMEM:STOR:TRAC 1, 'D:\rawdat.wv'"
```

' select RAW data export  
' select format waveform  
' start data export to file D:\rawdat.wv

**Characteristics:** \*RST value: ASCii  
SCPI: device-specific

## MMEMory subsystem

### MMEMory: LOAD:TRACe 1,<file\_name>

This command loads I/Q RAW data files. The file name includes indication of the path and the drive name. The path name complies with DOS conventions. This command is only available if RAW data with binary format is selected (":FORM:DEXP:MODE RAW", ":FORM:DEXP:RAW:FORM BIN"). The command needs two different files, created with the MMEM:STOR:TRAC command.

- <file\_name>.VAV VSA settings
- <file\_name>.bin I/Q RAW data

The import of the I/Q RAW data requires the MULTI mode to be active (refer to HOME VSA → MEAS RESULT → CAPTURE BUFFER → ZOOM → MULTI for more details). This mode is automatically switched on with start of the load process.

**Parameter:** <file\_name> ::= DOS file name

**Example:**

```

":INST:SEL DDEM"           ' enter VSA option
...                         ' additional commands to
...                         ' configure the measurement
                             ' and perform a measurement
":FORM:DEXP:MODE RAW"      ' select RAW data to export
":FORM:DEXP:RAW:FORM BIN"  ' select binary format
":MMEM:STOR:TRAC 1, 'D:\vsa_raw'" ' exports I/Q RAW data into
                             ' two files:
                             ' vsa_raw.vav (VSA settings)
                             ' vsa_raw.bin (I/Q RAW data)

"*RST"                     '
":INST:SEL DDEM"           ' enter VSA
":FORM:DEXP:MODE RAW"      ' select RAW data to import
":FORM:DEXP:RAW:FORM BIN"  ' select binary format
":MMEM:LOAD:TRAC 1, 'D:\vsa_raw'" ' import the I/Q RAW data files
                             ' vsa_raw.vav (VSA settings)
                             ' vsa_raw.bin (I/Q RAW data)

```

**Characteristics:** \*RST value: -  
SCPI: device-specific

This command is an event and therefore has no \*RST value and no query.

### MMEMory: STORE:TRACe 1,<file\_name>

This command stores I/Q RAW data files. The file name includes indication of path and drive name. The path name complies with DOS conventions. This command is only available if RAW data with binary format is selected (":FORM:DEXP:MODE RAW", ":FORM:DEXP:RAW:FORM BIN").

The import of the I/Q RAW data requires the MULTI mode to be active (refer to HOME VSA → MEAS RESULT → CAPTURE BUFFER → ZOOM → MULTI for more details). This mode is automatically switched on with start of the load process.

**Parameter:** <file\_name> ::= DOS file name

**Example:**

```

":INST:SEL DDEM"
...
...

":FORM:DEXP:MODE RAW"
":FORM:DEXP:RAW:FORM BIN"
":MMEM:STOR:TRAC 1, 'D:\vsa_raw'"
...

"*RST"
":INST:SEL DDEM"
":FORM:DEXP:MODE RAW"
":FORM:DEXP:RAW:FORM BIN"
":MMEM:LOAD:TRAC 1, 'D:\vsa_raw'"

```

**Characteristics:** \*RST value: -  
SCPI: device-specific

' enter VSA option  
' additional commands to  
' configure the measurement  
' and perform a measurement  
' select RAW data to export  
' select binary format  
' exports I/Q RAW data into  
' two files:  
' vsa\_raw.vav (VSA settings)  
' vsa\_raw.bin (I/Q RAW data)  
'  
' enter VSA  
' select RAW data to import  
' select binary format  
' import the I/Q RAW data file

This command is an event and therefore has no \*RST value and no query.

## SENSe subsystem

### :[SENSe<1|2>:]DDEMod:MAPPing:CATalog?

This command reads the available mappings for the selected modulation format stored on the hard disk. A mapping describes the assignment of constellation points to symbols.

The file names are output without file extension. Syntax of output format: mapping\_1, mapping\_2, ..., mapping\_n.

**Example:** ":DDEMod:MAPP:CAT?" ' queries the available mappings.

**Characteristics:** \*RST value: -  
SCPI: device-specific

### :[SENSe<1|2>:]DDEMod:PSK:FORMat NORMal | DIFFerential | D1Pi8 | N3Pi8

This command defines the specific demodulation mode for PSK. The specific demodulation mode (DDEMod:PSK:NST) must be set to 8.

The following PSK demodulation modes are possible:

DDEMod:PSK:NState	DDEMod:PSK:FORMat	Modulation mode
2	any	BPSK
8	NORMal	8PSK
8	DIFFerential	D8PSK
8	D1Pi8	$\pi/8$ -D8PSK
8	N3Pi8	$3\pi/8$ -8PSK (EDGE)

This command is only available for PSK demodulation.

**Example:** "DDEM:FORM PSK" ' Switch PSK demodulation  
' on.  
"DDEMod:PSK:NST 8"  
"DDEM:PSK:FORM DIFF" ' demodulation mode "  
' Switch D8PSK demodulation on

**Characteristics:** \*RST value: -  
SCPI: device-specific

**: [SENSe<1|2>: ]DDEMod:UQAM:FORMat '<UQAM\_demod\_mode>'**

This command selects the specific demodulation mode for User QAM.

The available User QAM demodulation modes are listed in the column USER-QAM of table MODULATION & MAPPING and depend on the contents of the available User QAM mapping files.

If several mappings are available for selected demodulation mode, it is additionally required to select the mapping to be used.

**Note:** ":SENS:DDEM:MAPP:CAT?" returns the available mappings for the currently selected demodulation mode.

This command is only available for User QAM demodulation.

**Parameter:** < UQAM\_demod\_mode > ' User QAM demodulation mode

**Example:** "DDEM:FORM UQAM" ' Switch User QAM demodulation  
' on.

"DDEM:UQAM:FORM 'UQAM\_demod\_mode'" ' Select the UQAM  
' demodulation mode

"DDEM:MAPP 'UQAM\_mapping\_file'" ' Select the User QAM mapping  
' if needed (see above)

**Characteristics:** \*RST value: -  
SCPI: device-specific

**: [SENSe<1|2>: ]DDEMod:UQAM:NSTate?**

This command returns the specific modulation level for User QAM.

This command is only available for User QAM demodulation.

**Parameter:** -

**Example:** "DDEM:FORM UQAM" ' Switch User QAM demodulation  
' on.

"DDEM:UQAM:FORM 'special'" ' Selects user mapping 'special'.

"DDEM: UQAM:NST?" ' returns the modulation level.

**Characteristics:** \*RST value: -  
SCPI: device-specific.

## Remote Control Commands - Programming Examples

The examples below show command sequences to be sent to the instrument or query commands to read data from the instrument. // indicates a comment and gives additional hints to the command used.

### Performing a Measurement with OPC Synchronization

```
*RST                                // reset instrument and enter VSA
INST:SEL DDEM                      // option
//
// Select a standard, change ConfigurePattern definition
//

:SENS:DDEM:PRES FW3G              // select standard 3G_WCDMA_FWD
:INIT:CONT OFF                    // Set to Single Sweep
                                   // required for OPC Sync and
                                   // improves configuration speed

:SENS:FREQ:CENT 1GHz              // Center Frequency 1GHz
:DISP:WIND:TRAC:Y:SCAL:RLEV -30.0 // Reference Level -30 dBm
//
// additional/other commands to configure the measurement
// ...
// ...
// Perform the measurement

:INIT:IMM;*OPC?                   // returns 1 when the sweep is
                                   // finished

// no results can be read from the instrument, e.g. marker, modulation
// summary,a.s.o.
```

### Creating a Search Pattern

The following command sequence defines a pattern "MY\_PAT" for a modulation with 16 states with bit sequence "111100001111000011110000".

The pattern is added to the standard NONE pattern list to be selectable in the Burst&Pattern selection dialog.

In addition, the QAM16 modulation is configured and the new pattern is selected to be used for the pattern search function and the pattern search is switched on.

The command "SENS:DDEM:SEAR:SYNC:CAT? ALL" lists all available pattern. The command "SENS:DDEM:SEAR:SYNC:CAT?" lists all pattern compatible to the current settings.

How to define the symbol sequence:

The bits has to be arranged as symbols. This depend on the number of states of the modulation, e.g. QAM16 has 16 possible states = 4bits/symbol:

Symbol sequence for a modulation with 16 states of the bit sequence above is:

"1111" = 000F hex

"0000" = 0000 hex

"1111" = 000F hex

"0000" = 0000 hex

"1111" = 000F hex

"0000" = 0000 hex

The command "SENS:DDEM:SEAR:SYNC:DATA" always expected a 4 character hex value for every symbol.

```
*RST                                // reset instrument and enter VSA
INST:SEL DDEM                       // option
//
// Pattern definition
//
SENS:DDEM:SEAR:SYNC:NAME    'MY_PAT'      // Select pattern name MY_PAT
SENS:DDEM:SEAR:SYNC:DEL      // delete old pattern, if it
                             // exists
SENS:DDEM:SEAR:SYNC:DATA    '000f0000000F0000000F0000' // always 4
                             // characters/symbol in HEX format
                             // 0000 ... 000F for QAM16 possible
SENS:DDEM:SEAR:SYNC:NST 16          // QAM16 has 16 states
SENS:DDEM:SEAR:SYNC:TEXT    'MY_PAT Selection' // This text will be visible
                             // after pressing SELECT PATTERN,
                             // dialog PATTERN SELECT (right
                             // column)
SENS:DDEM:SEAR:SYNC:COMM    'My Comment'   // Additional comment
//
// The pattern is now created and has to be added to the standard
// the pattern will be used for (Standard NONE here).
//
//      Select QAM16 modulation (-> Standard NONE)
//
:SENS:DDEM:FORM QAM
:SENSE1:DDEMod:QAM:NState 16
//
// This command queries all available patter, it is not required to
// define the pattern
SENS:DDEM:SEAR:SYNC:CAT? ALL          // returns all available pattern,
                                     // just to see the new pattern
                                     // exists now
:SENSE1:DDEMod:SEARch:SYNC:PATtern:ADD 'MY_PAT' // add the pattern MY_PAT
                                               // to standard NONE
                                               // now the new pattern is visible on
                                               // the pattern selection list for
                                               // standard NONE

:SENSE1:DDEMod:SEARch:SYNC:SEL 'MY_PAT' // select pattern MY_PAT for
                                         // pattern search
```

```
// switch pattern search ON
:SENSe1:DDEMod:SEARCh:SYNC:STATe ON           // activate the pattern search with
                                                // previously selected pattern
```

## Customer Support

### Technical support – where and when you need it

For quick, expert help with any Rohde & Schwarz equipment, contact one of our Customer Support Centers. A team of highly qualified engineers provides telephone support and will work with you to find a solution to your query on any aspect of the operation, programming or applications of Rohde & Schwarz equipment.

### Up-to-date information and upgrades

To keep your instrument up-to-date and to be informed about new application notes related to your instrument, please send an e-mail to the Customer Support Center stating your instrument and your wish. We will take care that you will get the right information.

#### Europe, Africa, Middle East

Phone +49 89 4129 12345  
[customersupport@rohde-schwarz.com](mailto:customersupport@rohde-schwarz.com)

#### North America

Phone 1-888-TEST-RSA (1-888-837-8772)  
[customer.support@rsa.rohde-schwarz.com](mailto:customer.support@rsa.rohde-schwarz.com)

#### Latin America

Phone +1-410-910-7988  
[customersupport.la@rohde-schwarz.com](mailto:customersupport.la@rohde-schwarz.com)

#### Asia/Pacific

Phone +65 65 13 04 88  
[customersupport.asia@rohde-schwarz.com](mailto:customersupport.asia@rohde-schwarz.com)