

**RSA6100A Series
Real-Time Spectrum Analyzers
Programmer Manual**



077-0249-01

Tektronix

**RSA6100A Series
Real-Time Spectrum Analyzers
Programmer Manual**

Copyright © Tektronix. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Contacting Tektronix

Tektronix, Inc.
14200 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
USA

For product information, sales, service, and technical support:

- In North America, call 1-800-833-9200.
- Worldwide, visit www.tektronix.com to find contacts in your area.

Table of Contents

Preface	v
Related Documentation	v

Getting Started

Getting Started	1-1
Overview of the Manual	1-1
Connecting the Interface	1-3
Using the GPIB Port	1-4
Setting the GPIB Address	1-5
Using TekVISA	1-6

Syntax and Commands

Command Syntax	2-1
Backus-Naur Form Definition	2-1
SCPI Commands and Queries	2-2
IEEE 488.2 Common Commands	2-8
Constructed Mnemonics	2-8
Command Groups	2-9
Measurement Views	2-9
Functional Groups	2-11
Programming Hints	2-12
IEEE Common Commands	2-13
Obsolete Commands	2-14
Abort Commands	2-15
Calculate Commands	2-16
Marker Mnemonics	2-24
Calibration Commands	2-25
Display Commands	2-26
Fetch Commands	2-35
Initiate Commands	2-43
Input Commands	2-44
Mass Memory Commands	2-45
Specifying the File	2-47

Output Commands.....	2-48
Read Commands.....	2-49
Sense Commands.....	2-57
Status Commands.....	2-69
System Commands.....	2-71
Trace Commands.....	2-72
Trace Mnemonics.....	2-75
Trigger commands.....	2-77
Unit Commands.....	2-79
Retrieving Response Message.....	2-80
Command Descriptions.....	2-81

Status and Events

Status and Events.....	3-1
Status and Event Reporting System.....	3-1
Status Byte.....	3-4
Standard Event Status Block.....	3-6
Operation Status Block.....	3-7
Questionable Status Block.....	3-8
Queues.....	3-10
Status and Event Processing Sequence.....	3-11
Synchronizing Execution.....	3-12
Error Messages and Codes.....	3-14
Command Errors.....	3-14
Execution Errors.....	3-15
Device Specific Errors.....	3-17
Query Errors.....	3-17
Device Errors.....	3-18
Status Conditions.....	3-21
Global Status.....	3-21
Measurement Status.....	3-21
Source Status.....	3-22

Appendices

Appendix A: Character Charts.....	A-1
Appendix B: GPIB Interface Specification.....	B-1
Interface Functions.....	B-1
Interface Messages.....	B-3

Appendix C: Factory Initialization Settings	C-1
Appendix D: SCPI Conformance Information	D-1

Glossary

Preface

This programmer manual covers the RSA6100A Series Real-Time Spectrum Analyzers. It provides information on operating your analyzer using the General Purpose Interface Bus (GPIB).

This manual is composed of the following sections

- *Getting Started* outlines how to use the GPIB interface.
- *Syntax and Commands* defines the syntax used in command descriptions, presents a list of all command subsystems, and presents detailed descriptions of all programming commands.
- *Status and Events* describes how the status and Events Reporting system operates and presents a list of all system errors.
- *Appendices* provides additional information including character charts, GPIB interface specification, and factory initialization settings.

Related Documentation

- *RSA6100A Series Quick Start User Manual*
(Tektronix part number 071-1909-XX)
This manual contains general information about how to put your instrument into service, guides to user interface controls, and application examples.
- *RSA6100A Series Online Help*
The online help contains detailed information about how to operate the instrument.
- *TekVISA Programmer Manual*
(Tektronix part number 071-1101-XX)
This manual is available as a printable PDF file on the Tektronix Web site (www.tektronix.com). The manual describes TekVISA, the Tektronix implementation of the VISA Application Programming Interface (API). TekVISA is industry-compliant software for writing interoperable instrument drivers in a variety of Application Development Environments (ADEs).

Getting Started

Getting Started

You can write computer programs that remotely set the analyzer front panel controls or that take measurements and read those measurements for further analysis or storage. To help you get started with programming the analyzer, this section includes the following subsections

- *Overview of the Manual*
Summarizes each major section of this manual.
- *Connecting the Interface*
Describes how to physically connect the analyzer to a controller.
- *Using GPIB Ports*
Describes how to use the GPIB port.
- *Setting the GPIB Address*
Describes how to set the GPIB parameters from the front panel.
- *Using TekVISA*
Describes how to use the TekVISA communication protocol.

Overview of the Manual

The information contained in each major section of this manual is described below.

Syntax and Commands

Syntax and Commands, describes the structure and content of the messages your program sends to the analyzer. The following figure shows command parts as described in the *Command Syntax* subsection.

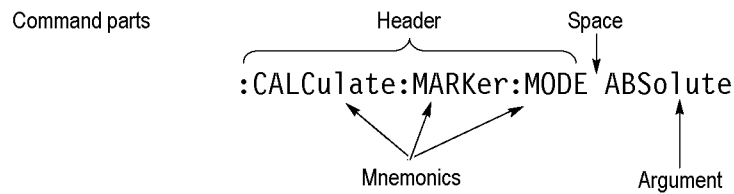


Figure 1-1: Command parts

Section 2 also describes the effect of each command and provides examples of how you might use it. The *Command Groups* subsection provides lists by functional areas. The commands are listed alphabetically in the *Command Descriptions* section.

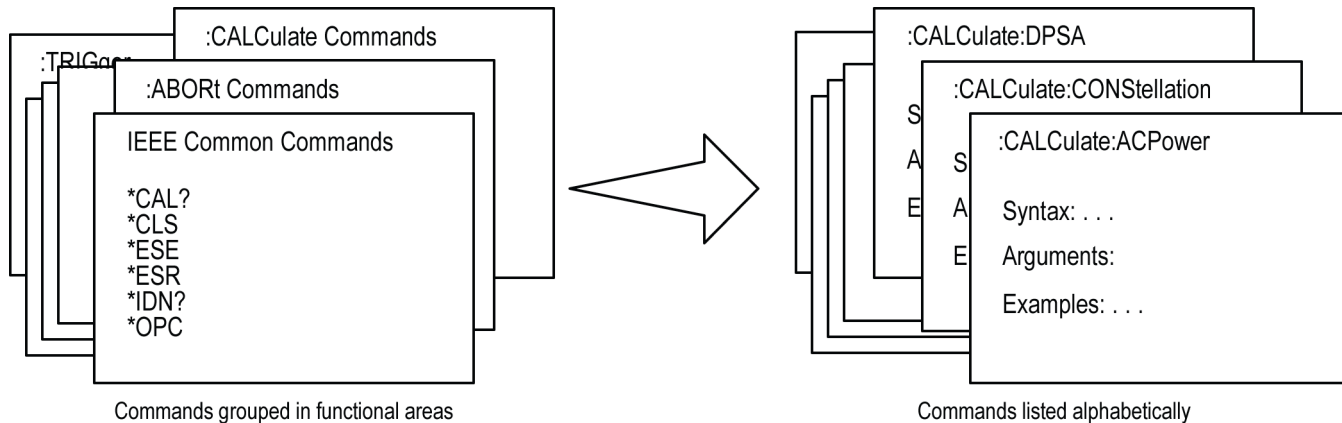


Figure 1-2: Functional groupings and an alphabetical list of commands

Status and Events

The program may request information from the instrument. The instrument provides information in the form of status and error messages. The following figure illustrates the basic operation of this system. Section 3, *Status and Events*, describes how to get status or event information from the program and details the event and error messages.

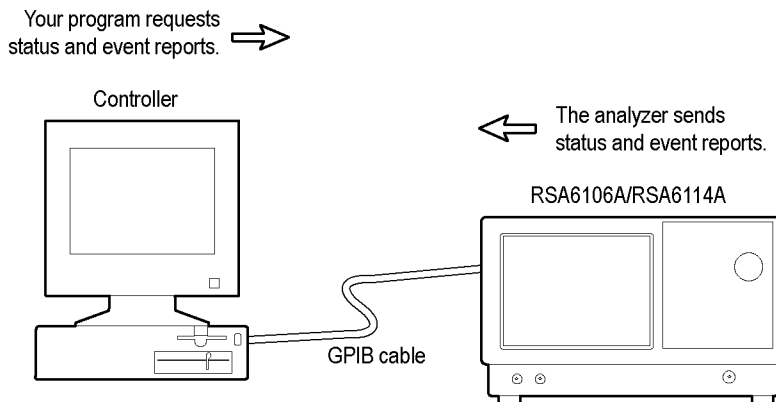


Figure 1-3: Event-driven program

Connecting the Interface

The instrument has a 24-pin GPIB connector on its rear panel, as shown in the following figure. This connector has a D-type shell and conforms to IEEE Std 488.1-1987. Attach an IEEE Std 488.1-1987 GPIB cable (Tektronix part number 012-0991-00) to this connector.

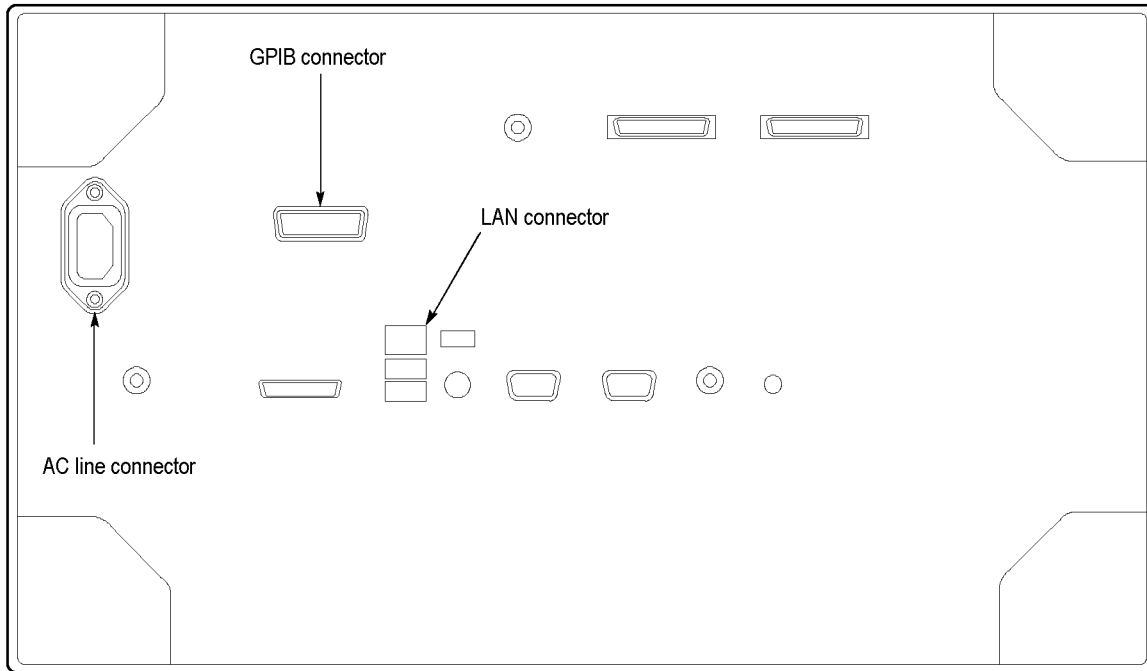


Figure 1-4: GPIB connector (rear panel)

Appendix B: GPIB Interface Specifications gives more information on the GPIB configuration of the analyzer. For the other interfaces, refer to the *RSA6100A Series Quick Start User Manual*.

Using the GPIB Port

The analyzer has Talker/Listener functions through which it can communicate with other devices, as well as the external controller, located on the bus.

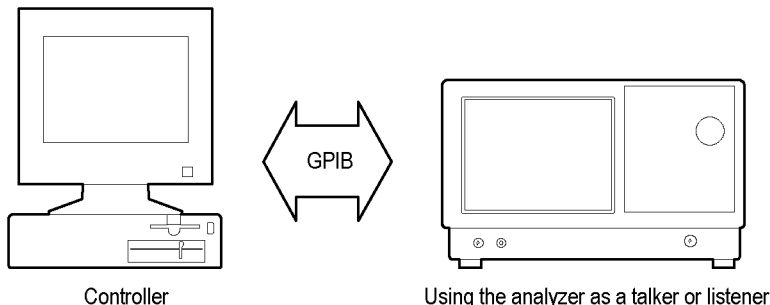


Figure 1-5: GPIB connection

GPIB Requirements

Observe the following rules when you use your analyzer with a GPIB network

- Assign a unique device address to each device on the bus. No two devices can share the same device address.
- Do not connect more than 15 devices to any one bus.
- Connect one device for every 2 m (6 ft) of cable used.
- Do not use more than 20 m (65 ft) of cable to connect devices to a bus.
- Turn on at least 2/3 of the devices on the network while using the network.
- Connect the devices on the network in a star or linear configuration, as shown in the following figure. Do not use loop or parallel configurations.


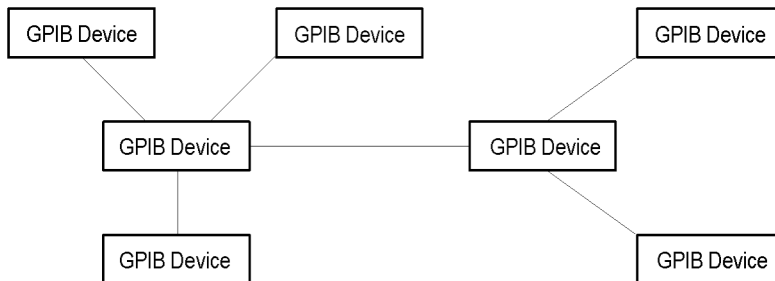


Figure 1-6: Typical GPIB network configurations


Setting the GPIB Address

When you use the GPIB port to communicate with an external controller, follow these steps to set the address of the analyzer.

1. From the **Tools** menu, select **Options** to open the Options control panel.

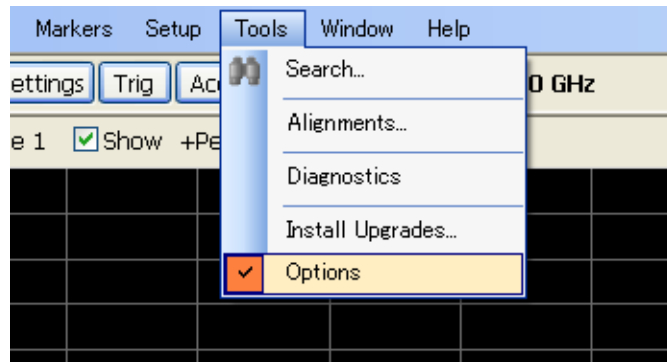

2. Click the **GPIB** tab and set the primary address. Range: 0 to 30 (default: 1)

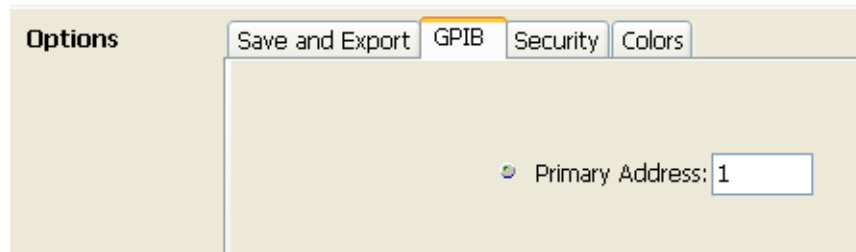

NOTE. The GPIB address cannot be initialized by the *RST command.

Using TekVISA

TekVISA is Tektronix implementation of VISA (Virtual Instrument Software Architecture), an industry-standard communication protocol. VISA provides a common standard for software developers so that software from multiple vendors, such as instrument drivers, can run on the same platform. TekVISA is industry-compliant software, available with selected Tektronix instruments. You can use this software to write (or draw) interoperable instrument drivers in a variety of Application Development Environments (ADEs). It implements a subset of Version 2.2 of the VISA specification for controlling GPIB and serial (RS-232) instrument interfaces locally or remotely via an Ethernet LAN connection.

Installation

Use an internet browser to access the Tektronix Web site (www.tektronix.com) and download the current TekVISA to your PC. Unzip the downloaded file in a temporary directory of your choice and run *Setup.exe*.

NOTE. *The details on TekVISA concepts and operations are explained in the TekVISA Programmer Manual that can be also found on the Tektronix Web site.*

Syntax and Commands

Command Syntax

This section contains information on the Standard Commands for Programmable Instruments (SCPI) and IEEE 488.2 Common Commands you can use to program your RSA6106A/RSA6114A analyzer. The information is organized in the following subsections

- Backus-Naur Form Definition
- SCPI Commands and Queries
- IEEE 488.2 Common Commands
- Constructed Mnemonics

Backus-Naur Form Definition

This manual may describe commands and queries using the Backus-Naur Form (BNF) notation. The following table defines the standard BNF symbols.

Table 2-1: BNF symbols and meanings

Symbol	Meaning
< >	Defined element
:=	Is defined as
	Exclusive OR
{ }	Group; one element is required
[]	Optional; can be omitted
... .	Previous element(s) may be repeated
()	Comment

SCPI Commands and Queries

SCPI is a standard created by a consortium that provides guidelines for remote programming of instruments. These guidelines provide a consistent programming environment for instrument control and data transfer. This environment uses defined programming messages, instrument responses, and data format across all SCPI instruments, regardless of manufacturer. The analyzer uses a command language based on the SCPI standard.

The SCPI language is based on a hierarchical or tree structure as shown in the following figure that represents a subsystem. The top level of the tree is the root node; it is followed by one or more lower-level nodes.

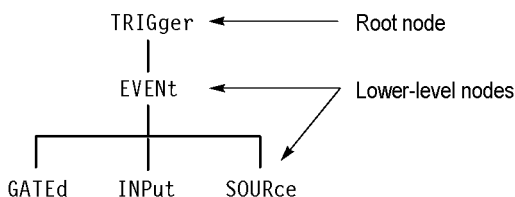


Figure 2-1: Example of SCPI subsystem hierarchy tree

You can create commands and queries from these subsystem hierarchy trees. Commands specify actions for the instrument to perform. Queries return measurement data and information about parameter settings.

Creating Commands

SCPI commands are created by stringing together the nodes of a subsystem hierarchy and separating each node by a colon.

In the figure above, TRIGger is the root node and EVENTt, GATEd, INPut, and SOURce are lower-level nodes. To create a SCPI command, start with the root node TRIGger and move down the tree structure adding nodes until you reach the end of a branch. Most commands and some queries have parameters; you must include a value for these parameters. If you specify a parameter value that is out of range, the parameter will be set to a default value. The command descriptions, list the valid values for all parameters.

For example, TRIGgerEVENTt:SOURce EXTRear is a valid SCPI command created from the hierarchy tree. (See Figure 2-1.)

Creating Queries

To create a query, start at the root node of a tree structure, move down to the end of a branch, and add a question mark. TRIGgerEVENTt:SOURce? is an example of a valid SCPI query using the hierarchy tree in the figure. (See Figure 2-1.)

Query Responses

The query causes the analyzer to return information about its status or settings. When a query is sent to the analyzer, only the values are returned. When the returned value is a mnemonic, it is noted in abbreviated format, as shown in the following table.

Table 2-2: Query response examples

Query	Response
CALCulate:SPECtrum:MARKer:X	7.50E+9
SENSe:SPECtrum:FFT:WINDow	BH4B

A few queries also initiate an operation action before returning information. For example, the *CAL? query runs a calibration.

Parameter Types

Every parameter in the command and query descriptions is of a specified type. The parameters are enclosed in brackets, such as <value>. The parameter type is listed after the parameter and is enclosed in parentheses, for example, (boolean). Some parameter types are defined specifically for the RSA6100A Series command set and some are defined by ANSI/IEEE 488.2-1987 as shown in the following table.

Table 2-3: Parameter types used in syntax descriptions

Parameter type	Description	Example
arbitrary block ¹	A specified length of arbitrary data	#512234xxxx . . . where 5 indicates that the following 5 digits (12234) specify the length of the data in bytes; xxxx ... indicates the data
boolean	Boolean numbers or values	ON or 1; OFF or 0
binary	Binary numbers	#B0110
octal	Octal numbers	#Q57, #Q3
hexadecimal ²	Hexadecimal numbers (0-9, A, B, C, D, E, F)	#HAA, #H1
NR1 ² numeric	Integers	0, 1, 15, -1
NR2 ^{2,3} numeric	Decimal numbers	1.2, 3.141516, -6.5
NR3 ² numeric	Floating point numbers	3.1415E-9, -16.1E5
NRf ² numeric	Flexible decimal number that may be type NR1, NR2 or NR3	See NR1, NR2, and NR3 examples
string ⁴	Alphanumeric characters (must be within quotation marks)	"Testing 1, 2, 3"

¹ Defined in ANSI/IEEE 488.2 as "Definite Length Arbitrary Block Response Data."

² An ANSI/IEEE 488.2-1992-defined parameter type.

³ Some commands and queries will accept an octal or hexadecimal value even though the parameter type is defined as NR1.

⁴ Defined in ANSI/IEEE 488.2 as "String Response Data."

Chaining Commands and Queries

You can chain several commands or queries together into a single message. To create a chained message, first create a command or query, add a semicolon (;), and then add more commands or queries and semicolons until the message is complete. If the command following a semicolon is a root node, precede it with a colon (:). The following figure illustrates a chained message consisting of several commands and queries. The single chained message should end in a command or query, not a semicolon. Responses to any queries in your message are separated by semicolons.


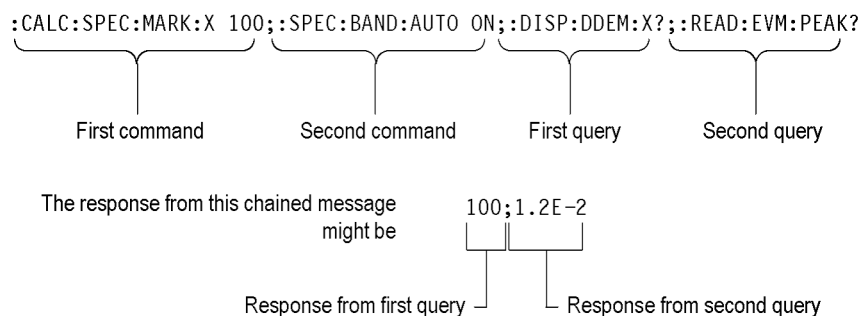


Figure 2-3: Example of chaining commands and queries

If a command or query has the same root and lower-level nodes as the previous command or query, you can omit these nodes. In the following figure, the second command has the same root node (TRIGgerEVENT) as the first command, so these nodes can be omitted.

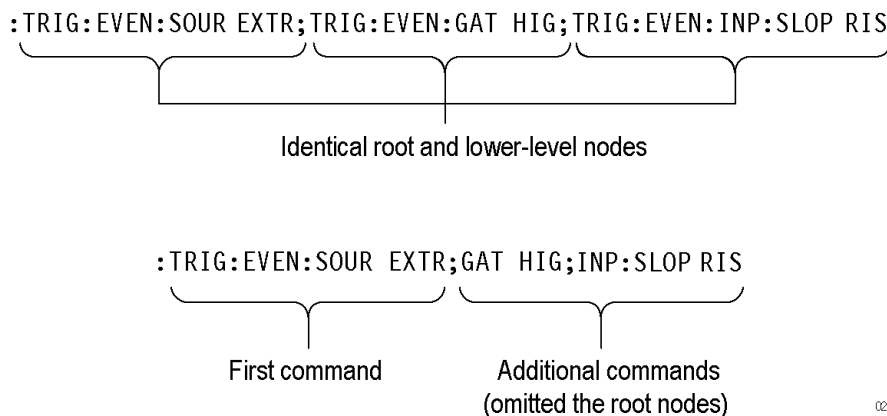

0249-001

Figure 2-4: Example of omitting root and lower-level nodes in a chained message

Unit and SI Prefix

If the decimal numeric argument refers to amplitude, frequency, or time, you can express it using SI units instead of using the scaled explicit point input value format <NR3>. (SI units are units that conform to the Systeme International d'Unites standard.) For example, you can use the input format 200 mV or 1.0 MHz instead of 200.0E-3 or 1.0E+6, respectively, to specify voltage or frequency.

The following table lists the available units.

Table 2-4: Available units

Symbol	Meaning
dB	decibel (relative amplitude)
dBm	decibel (absolute amplitude)
DEG	degree (phase)
Hz	hertz (frequency)
PCT	percent (%)
s	second (time)
V	volt

The available SI prefixes are shown in the following table.

Table 2-5: Available SI prefixes

SI prefix	Z	A	F	P	N	U	M	K	MA ¹	G	T	PE	EX
Corresponding power	10 ⁻²¹	10 ⁻¹⁸	10 ⁻¹⁵	10 ⁻¹²	10 ⁻⁹	10 ⁻⁶	10 ⁻³	10 ⁺³	10 ⁺⁶	10 ⁺⁹	10 ⁺¹²	10 ⁺¹⁵	10 ⁺¹⁸

¹ When the unit is "Hz", "M" may be used instead of "MA" so that the frequency can be represented by "MHz".

You can omit a unit in a command, but you must include the unit when using a SI prefix. For example, frequency of 15 MHz can be described as follows

15.0E6, 1.5E7Hz, 15000000, 15000000Hz, 15MHz, etc.
("15M" is not allowed.)

Note that you can use either lower or upper case units and prefixes. The following examples have the same result, respectively.

170mhz, 170mHz, 170MHz, etc.
250mv, 250mV, 250MV, etc.

General Rules

Here are three general rules for using SCPI commands, queries, and parameters:

- You can use single (‘ ’) or double (“ ”) quotation marks for quoted strings, but you cannot use both types of quotation marks for the same string.

correct "This string uses quotation marks correctly."

correct ‘This string also uses quotation marks correctly.’

incorrect "This string does not use quotation marks correctly.’

- You can use upper case, lower case, or a mixture of both cases for all commands, queries, and parameters.

SENSE:SPECTRUM:FFT:LENGTH 1024

is the same as

sense:spectrum:fft:length 1024

and

SENSE:spectrum:FFT:length 1024

NOTE. *Literal strings (quoted) are case sensitive, for example, file names.*

- No embedded spaces are allowed between or within nodes.

correct SENSE:SPECTRUM:FFT:LENGTH 1024

incorrect SENSE: SPECTRUM: FFT: LEN GTH 1024

IEEE 488.2 Common Commands

Description	ANSI/IEEE Standard 488.2 defines the codes, formats, protocols, and usage of common commands and queries used on the interface between the controller and the instruments. The analyzer complies with this standard.
Command and Query Structure	<p>The syntax for an IEEE 488.2 common command is an asterisk (*) followed by a command and, optionally, a space and parameter value. The syntax for an IEEE 488.2 common query is an asterisk (*) followed by a query and a question mark. All of the common commands and queries are listed in the last part of the <i>Syntax and Commands</i> section. The following are examples of common commands:</p> <ul style="list-style-type: none"> ■ *ESE 16 ■ *CLS <p>The following are examples of common queries</p> <ul style="list-style-type: none"> ■ *ESR ■ *IDN

Constructed Mnemonics

Some header mnemonics specify one of a range of mnemonics. For example, a trace mnemonic can be either TRACe1, TRACe2, TRACe3, or TRACe4. You use these mnemonics in the command just as you do any other mnemonic. For example, there is a TRACe1:SPECTrum:FUNCTion command, and there is also a TRACe2:SPECTrum:FUNCTion command. In the command descriptions, this list of choices is abbreviated as TRACe<x>. The value of <x> is the upper range of valid suffixes. If the numeric suffix is omitted, the analyzer uses the default value of "1".

Table 2-6: Constructed mnemonics

Symbol	Meaning
MARKer<x>	A marker specifier where <x> = 0, 1, 2, 3, or 4. Refer to <i>Marker Mnemonics</i>
RANGe<x>	A range specifier where <x> = 1 to 20. Refer to <i>[SENSe]:SPURious Subgroup</i> for details.
SPUR<x>	A spurious specifier where <x> = 1 to the number of spurious signals. Refer to <i>FETCh :READ:SPURious Subgroup</i> for details, respectively.
TRACe<x>	A trace specifier where <x> = 0, 1, 2, 3, 4, or 5. Refer to <i>TRACe Commands</i> for details.

Command Groups

This section lists the RSA6100A Series analyzer commands in two ways. It first presents them by functional groups. It then lists them alphabetically. The functional group list starts below. The alphabetical list provides more detail on each command.

The RSA6100A Series analyzers conform to the Standard Commands for Programmable Instruments (SCPI) 1999.0 and IEEE Std 488.2-1987 except where noted.

Items followed by question marks are queries; items without question marks are commands. Some items in this section have a question mark in parentheses () in the command header section; this indicates that the item can be both a command and a query.

For the conventions of notation in this manual, refer to *Command Syntax* and following pages.

Measurement Views

The measurement views in the RSA6100A Series analyzers are categorized into the following five groups:

- General signal viewing
- General purpose analog demodulation (Option 21 only)
- General purpose digital modulation (Option 21 only)
- RF measurements
- Pulsed RF (Option 20 only)

Each group contains the measurement views as shown in the following table. Each command works in particular measurement view(s) which are specified under the *Conditions* heading in the command descriptions.

NOTE. *If you send a command for the measurement view that is not displayed on screen, an execution error will occur.*

Table 2-7: Measurement views

Display group	Measurement view
General signal viewing	Spectrum
	DPX (Digital Phosphor) spectrum
	Amplitude versus Time
	Frequency versus Time
	Phase versus Time
	RF I&Q versus Time
	Spectrogram
General purpose analog demodulation (Option 21 only)	Time overview
	AM
	FM
General purpose digital modulation (Option 21 only)	PM
	Constellation
	Demodulated I&Q vs Time
	EVM versus Time
	Eye diagram
	Frequency deviation vs Time
	Magnitude error versus Time
	Phase error versus Time
	Signal quality
	Symbol table
RF measurements	Trellis diagram
	CCDF
	Channel power and ACPR (Adjacent Channel Power Ratio)
	MCPR (Multiple Carrier Power Ratio)
	Occupied Bandwidth (OBW)
	Phase noise (Option 11 only)
	Spurious
Pulsed RF (Option 20 only)	Pulse statistics
	Pulse table
	Pulse trace

Functional Groups

All commands are divided into groups as shown in the following table.

Table 2-8: List of command group

Command group	Function
IEEE common	Conforms to the IEEE Std 488.2.
ABORt	Resets the trigger system and stops measurements.
CALCulate	Controls the markers and the search operations.
CALibration	Controls the external correction.
DISPlay	Controls the display of measurement results and waveforms.
FETCh	Retrieves the measurements from the last acquired data.
INITiate	Controls data acquisition.
INPut	Controls the characteristics of the signal input.
MMEMory	Provides mass storage capabilities for the analyzer.
OUTPut	Controls the characteristics of the signal output.
READ	Obtains the measurement results with acquiring data.
SENSe	Sets up detailed conditions for each measurement.
STATus	Controls the status and event registers.
SYSTem	Sets or queries system parameters for operation.
TRACe	Controls trace activation and math operations.
TRIGger	Controls triggering.
UNIT	Specifies fundamental units for measurement.

Programming Hints

Here are some basic tips for using the RSA6100A Series GPIB commands:

- *Selecting a measurement item*
Use Display commands to select or display the measurement view.
[Example] `DISPlay:GENeral:MEASview:NEW SPECTrum`
Displays the spectrum view on the screen.
- *Setting measurement parameters*
Use Sense commands to set conditions for the measurement session.
[Example] `SENSe:SPECTrum:FREQUENCY:CENTer 1.5GHZ`
Sets the center frequency to 1.5 GHz in the spectrum view.
- *Acquiring an input signal*
Use an Initiate or Abort command to start or stop data acquisition.
[Example] `INITiate:CONTinuous ON;INITiate:IMMediate`
Starts data acquisition in the continuous mode.
- *Processing waveforms arithmetically*
Use Trace commands for math operation on waveforms.
[Example] `TRACe1:SPECTrum:FUNCTion`
`AVERage` Averages the spectrum waveform.
- *Measuring with the markers*
Use Calculate commands to measure some quantity using the markers.
[Example] `CALCulate:SPECTrum:MARKer1:MAXimum`
Positions the marker at the highest peak signal on the spectrum.
- *Obtaining the measurement results*
Use a Fetch or Read command to get the results.
[Example] `FETCH:SPECTrum:TRACe1`
Returns the spectrum trace data.
- *Scaling the waveform*
Use Display commands to change the waveform portion on screen.
[Example] `DISPlay:IQVTime:Y:SCALE 1.5`
Sets the vertical range to 1.5 V in the IQ versus Time graph.

Refer to *Appendix C* for the default settings of the commands. (See page 3-1.)

The following sections list the commands by group.

IEEE Common Commands

The IEEE 488.2 common commands have a "*" prefix.

Table 2-9: Status and error commands

Header	Description
*CAL	Performs an internal self-calibration.
*CLS	Clears status.
*ESE	Sets or queries the bits in the ESER register.
*ESR?	Returns the contents of the SESR register.
*IDN?	Returns the instrument identification code.
*OPC	Synchronizes commands.
*OPT?	Returns a list of options installed in your analyzer.
*RST	Returns the instrument settings to the factory defaults.
*SRE	Sets or queries the bits in the SRER register.
*STB?	Returns the contents of the SBR using the MSS bit.
*TRG	Generates a trigger.
*WAI	Prevents the analyzer from executing further commands.

Obsolete Commands

The following table lists obsolete commands and their replacements.

Table 2-10: Obsolete and replacement commands

Obsolete commands	Replacement commands
[SENSe:]PULSe:ANALyze:MEASurement:TIME:AUTO	[SENSe:]PULSe:ANALyze:FDOMain:MEASurement:TIME:ALENght
[SENSe:]PULSe:ANALyze:MEASurement:TIME:START	[SENSe:]PULSe:ANALyze:FDOMain:MEASurement:TIME:METHod
[SENSe:]PULSe:ANALyze:MEASurement:TIME:STOP	[SENSe:]PULSe:ANALyze:FDOMain:MEASurement:TIME:RLENght
	[SENSe:]PULSe:ANALyze:FDOMain:MEASurement:TIME:RLEVel
	[SENSe:]PULSe:ANALyze:FDOMain:MEASurement:TIME:START
	[SENSe:]PULSe:ANALyze:IRESponse:MEASurement:TIME:
	ALENght
	[SENSe:]PULSe:ANALyze:IRESponse:MEASurement:TIME:
	METHod
	[SENSe:]PULSe:ANALyze:IRESponse:MEASurement:TIME:
	RLENght
	[SENSe:]PULSe:ANALyze:IRESponse:MEASurement:TIME:RLEVel
	[SENSe:]PULSe:ANALyze:IRESponse:MEASurement:TIME:START
	[SENSe:]PULSe:ANALyze:OVERshoot:MEASurement:TIME:
	ALENght
	[SENSe:]PULSe:ANALyze:OVERshoot:MEASurement:TIME:
	METHod
	[SENSe:]PULSe:ANALyze:OVERshoot:MEASurement:TIME:
	RLENght
	[SENSe:]PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEVel
	[SENSe:]PULSe:ANALyze:OVERshoot:MEASurement:TIME:START
[SENSe:]PULSe:FREFerence:CHIRpbw(?)	[SENSe:]PULSe:FREFerence:CSLope

Abort Commands

Use the Abort commands to reset the trigger system and to stop measurements.

Table 2-11: Abort commands

Header	Description
ABORt	Resets the trigger system and stops measurements.

Calculate Commands

Use the Calculate commands to control the markers and the search operations.

Table 2-12: Calculate commands

Header	Description
CALCulate basic command subgroup	General marker control
CALCulate:MARKer:ADD	Adds a marker.
CALCulate:MARKer:AOff	Turns off all markers.
CALCulate:MARKer:DELeTe	Deletes the last marker added.
CALCulate:MARKer:DENSity:EXCursion	Sets or queries the minimum excursion of DPX signal density.
CALCulate:MARKer:DENSity:SMOothing	Sets or queries the number of pixels squared for smoothing the density.
CALCulate:MARKer:DENSity:THReshold	Sets or queries the threshold of DPX signal density to detect peaks.
CALCulate:MARKer:MODE	Sets or queries the marker mode.
CALCulate:MARKer:PEAK:EXCursion	Sets or queries the minimum excursion level.
CALCulate:MARKer:PEAK:THReshold	Sets or queries the threshold level to detect peaks.
CALCulate:SEARch:LIMit:FAIL?	Queries whether the waveform cuts across the limit or not.
CALCulate:SEARch:LIMit:MATCH:BEEP[:STATe]	Sets or queries whether to beep when a match occurs.
CALCulate:SEARch:LIMit:MATCH:SACQuire[:STATe]	Sets or queries whether to stop acquiring data on match.
CALCulate:SEARch:LIMit:MATCH:SDATa[:STATe]	Sets or queries whether to save the acquisition data automatically.
CALCulate:SEARch:LIMit:MATCH:SPICture[:STATe]	Sets or queries whether to save the whole screen automatically.
CALCulate:SEARch:LIMit:MATCH:STRace[:STATe]	Sets or queries whether to save the spectrum trace automatically.
CALCulate:SEARch:LIMit:OPERation	Sets or queries the limit operation in the search function.
CALCulate:SEARch:LIMit:OPERation:FEED	Sets or queries the data flow to be fed in the search operation.
CALCulate:SEARch:LIMit:OPERation:MASK:LOAD	Loads the limit mask from a specified file for the search operation.
CALCulate:SEARch:LIMit:OPERation:MASK:STORE	Stores the limit mask to a specified file for the search operation.
CALCulate:SEARch:LIMit:OPERation:SLIMit	Sets or queries the limit value in the search operation.
CALCulate:SEARch:LIMit:REPort:DATA?	Returns the frequency range(s) that satisfy the search condition.
CALCulate:SEARch:LIMit:REPort:POINts?	Returns the number of range(s) that satisfy the search condition.
CALCulate:SEARch:LIMit:STATe	Sets or queries whether to enable or disable the search function.
CALCulate:ACPower subgroup	Channel power and ACPR measurement
CALCulate:ACPower:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
CALCulate:ACPower:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:ACPower:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:ACPower:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:ACPower:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:ACPower:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:ACPower:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.

Table 2-12: Calculate commands (cont.)

Header	Description
CALCulate:{AM FM PM} subgroup (Option 21 only)	AM/FM/PM measurement
CALCulate:{AM FM PM}:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
CALCulate:{AM FM PM}:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:{AM FM PM}:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:{AM FM PM}:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:{AM FM PM}:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:{AM FM PM}:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:{AM FM PM}:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:{AM FM PM}:MARKer<x>:X	Sets or queries the horizontal position (time) of the marker.
CALCulate:{AM FM PM}:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:AVTime subgroup	Frequency versus Time measurement
CALCulate:AVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
CALCulate:AVTime:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:AVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:AVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:AVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:AVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:AVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:AVTime:MARKer<x>:TRACe	Sets or queries the trace on which the marker is placed.
CALCulate:AVTime:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:AVTime:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:CONSte subgroup (Option 21 only)	Constellation measurement
CALCulate:CONSte:MARKer<x>:DELTA:X[:TIME]?	Returns the delta marker time for the selected marker.
CALCulate:CONSte:MARKer<x>:FDEVIation?	Queries the frequency deviation of the selected marker.
CALCulate:CONSte:MARKer<x>:MAGNitude?	Queries the magnitude readout of the marker.
CALCulate:CONSte:MARKer<x>:MAXimum	Positions the marker at the symbol in the center of the time record.
CALCulate:CONSte:MARKer<x>:PEAK:LEFT	Moves the marker in the time domain to the next lower symbol number.
CALCulate:CONSte:MARKer<x>:PEAK:RIGHT	Moves the marker in the time domain to the next higher symbol number.
CALCulate:CONSte:MARKer<x>:PHASe?	Queries the phase readout of the marker.
CALCulate:CONSte:MARKer<x>:SYMBol?	Queries the symbol readout of the marker.
CALCulate:CONSte:MARKer<x>:VALue?	Queries the value readout of the marker.
CALCulate:CONSte:MARKer<x>:X	Sets or queries the time position of the marker on the trace.
CALCulate:DIQVtime subgroup (Option 21 only)	Demodulated I&Q versus Time measurement
CALCulate:DIQVtime:MARKer<x>:DELTA:X[:TIME]?	Returns the delta marker time for the selected marker.
CALCulate:DIQVtime:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:DIQVtime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:DIQVtime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.

Table 2-12: Calculate commands (cont.)

Header	Description
CALCulate:DIQVtime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:DIQVtime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:DIQVtime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:DIQVtime:MARKer<x>:TRACe	Places the selected marker on the Demodulated I&Q versus Time trace.
CALCulate:DIQVtime:MARKer<x>:X[:TIME]	Sets or queries the horizontal position (time) of the marker.
CALCulate:DIQVtime:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:DPSA subgroup	DPX spectrum measurement
CALCulate:DPSA:MARKer<x>:DELTA:X:AMPLitude?	Returns the delta marker amplitude for the selected marker.
CALCulate:DPSA:MARKer<x>:DELTA:X[:FREQuency]?	Returns the delta marker frequency for the selected marker.
CALCulate:DPSA:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:DPSA:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:DPSA:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:DPSA:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:DPSA:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:DPSA:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:DPSA:MARKer<x>[:SET]:CENTer	Sets the center frequency to the marker frequency.
CALCulate:DPSA:MARKer<x>:TRACe	Sets or queries the trace to attach the marker to.
CALCulate:DPSA:MARKer<x>:X:AMPLitude	Sets or queries the amplitude position of the marker.
CALCulate:DPSA:MARKer<x>:X[:FREQuency]	Sets or queries the frequency position of the marker.
CALCulate:DPSA:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:EDIagram subgroup (Option 21 only)	Eye diagram
CALCulate:EDIagram:MARKer<x>:DELTA:X[:TIME]?	Returns the delta marker time for the selected marker.
CALCulate:EDIagram:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:EDIagram:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:EDIagram:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:EDIagram:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:EDIagram:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:EDIagram:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:EDIagram:MARKer<x>:TRACe	Places a marker on the I or Q trace in the eye diagram display.
CALCulate:EDIagram:MARKer<x>:X[:TIME]	Sets or queries the horizontal position (time) of the marker.
CALCulate:EDIagram:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:EVM subgroup (Option 21 only)	EVM versus Time measurement
CALCulate:EVM:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
CALCulate:EVM:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:EVM:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:EVM:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:EVM:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.

Table 2-12: Calculate commands (cont.)

Header	Description
CALCulate:EVM:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:EVM:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:EVM:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:EVM:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:FDVTime subgroup (Option 21 only)	Frequency deviation versus Time measurement
CALCulate:FDVTime:MARKer<x>:DELTA:X[:TIME]?	Returns the delta marker time for the selected marker.
CALCulate:FDVTime:MARKer<x>:DELTA:Y?	Returns the delta marker frequency for the selected marker.
CALCulate:FDVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:FDVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:FDVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:FDVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:FDVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:FDVTime:MARKer<x>:X[:TIME]	Sets or queries the horizontal position (time) of the marker.
CALCulate:FDVTime:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:FVTime subgroup	Frequency versus Time measurement
CALCulate:FVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
CALCulate:FVTime:MARKer<x>:DELTA:Y?	Returns the delta marker frequency for the selected marker.
CALCulate:FVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:FVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:FVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:FVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:FVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:FVTime:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:FVTime:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:IQVTime subgroup	RF I&Q versus Time measurement
CALCulate:IQVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
CALCulate:IQVTime:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:IQVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:IQVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:IQVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:IQVTime:MARKer<x>:TRACe	Sets or queries the trace (I or Q) to place the marker.
CALCulate:IQVTime:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:IQVTime:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:MCPower subgroup	MCPR measurement
CALCulate:MCPower:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.

Table 2-12: Calculate commands (cont.)

Header	Description
CALCulate:MCPower:MARKer<x>:DELta:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:MCPower:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:MCPower:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:MCPower:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:MCPower:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:MCPower:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
CALCulate:MERRor:MARKer<x>:DELta:X?	Returns the delta marker time for the selected marker.
CALCulate:MERRor:MARKer<x>:DELta:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:MERRor:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:MERRor:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:MERRor:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:MERRor:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:MERRor:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:MERRor:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:MERRor:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:OBWidth subgroup	Occupied Bandwidth measurement
CALCulate:OBWidth:MARKer<x>:DELta:X?	Returns the delta marker frequency for the selected marker.
CALCulate:OBWidth:MARKer<x>:DELta:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:OBWidth:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:OBWidth:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:OBWidth:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:OBWidth:MARKer<x>[:SET]:CENTer	Sets the center frequency to the value at the marker position.
CALCulate:OBWidth:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:OBWidth:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
CALCulate:PERRor:MARKer<x>:DELta:X?	Returns the delta marker time for the selected marker.
CALCulate:PERRor:MARKer<x>:DELta:Y?	Returns the delta marker phase for the selected marker.
CALCulate:PERRor:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:PERRor:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:PERRor:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:PERRor:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:PERRor:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:PERRor:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:PERRor:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.

Table 2-12: Calculate commands (cont.)

Header	Description
CALCulate:PHVTime subgroup	Phase versus Time measurement
CALCulate:PHVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
CALCulate:PHVTime:MARKer<x>:DELTA:Y?	Returns the delta marker phase for the selected marker.
CALCulate:PHVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:PHVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:PHVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:PHVTime:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:PHVTime:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:PULSe subgroup (Option 20 only)	Pulsed RF measurements
CALCulate:PULSe:STATistics:FFT:INDicator:X	Sets or queries the frequency in Hz for the X cursor.
CALCulate:PULSe:STATistics:FFT:INDicator:Y?	Returns the frequency level in dB for the Y cursor.
CALCulate:PULSe:STATistics:HISTogram:INDicator:X	Sets or queries the histogram indicator X value.
CALCulate:PULSe:STATistics:HISTogram:INDicator:Y?	Queries the histogram indicator Y value.
CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the specified marker.
CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the specified marker.
CALCulate:PULSe:STATistics:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:PULSe:STATistics:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the statistics trace.
CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:PULSe:STATistics:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the statistics trace.
CALCulate:PULSe:STATistics:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:PULSe:STATistics:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:PULSe:TRACe:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
CALCulate:PULSe:TRACe:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:PULSe:TRACe:MARKer<x>:MAXimum	Moves the marker to the highest peak on the pulse trace.
CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the pulse trace.
CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the pulse trace.
CALCulate:PULSe:TRACe:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:PULSe:TRACe:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:SEARCh subgroup	Spectrogram measurement
CALCulate:SEARCh:LIMit:FAIL?	Queries whether the waveform cuts across the limit in the search operation.

Table 2-12: Calculate commands (cont.)

Header	Description
CALCulate:SEARch:LIMit:MATCh:BEEP[:STATe]	Sets or queries whether or not to emit a beep on match during run or replay in the search operation.
CALCulate:SEARch:LIMit:MATCh:SACQuire[:STATe]	Sets or queries whether or not to stop acquiring data on match during run or replay in the search operation.
CALCulate:SEARch:LIMit:MATCh:SDATa[:STATe]	Sets or queries whether or not to save automatically (AutoSave) acquisition data on match during run in the search operation.
CALCulate:SEARch:LIMit:MATCh:SPICture[:STATe]	Sets or queries whether or not to save automatically (AutoSave) the whole screen on match during run in the search operation.
CALCulate:SEARch:LIMit:MATCh:STRace[:STATe]	Sets or queries whether or not to save automatically (AutoSave) the spectrum trace on match during run in the search operation.
CALCulate:SEARch:LIMit:OPERation	Sets or queries the search condition parameter.
CALCulate:SEARch:LIMit:OPERation:FEED	Sets or queries the data flow to be fed in the search operation.
CALCulate:SEARch:LIMit:OPERation:MASK:LOAD	Loads the specified limit mask file for the search operation.
CALCulate:SEARch:LIMit:OPERation:MASK:STORE	Saves the limit mask to a specified file.
CALCulate:SEARch:LIMit:OPERation:SLIMit	Sets or queries the limit value (in dB) in the search operation.
CALCulate:SEARch:LIMit:REPort:DATA?	Queries the frequency range(s) that satisfy the search condition.
CALCulate:SEARch:LIMit:REPort:POINts?	Queries the number of frequency range(s) that satisfy the search condition.
CALCulate:SEARch:LIMit:STATe	Sets or queries the search function (enabled or disabled).
CALCulate:SGRam subgroup	Spectrogram measurement
CALCulate:SGRam:MARKer<x>:DELTA:X:FREQuency?	Returns the delta marker frequency for the selected marker.
CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]?	Returns the delta marker time for the selected marker.
CALCulate:SGRam:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:SGRam:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:SGRam:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:SGRam:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:SGRam:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:SGRam:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:SGRam:MARKer<x>[:SET]:CENTer	Sets the center frequency to the marker frequency.
CALCulate:SGRam:MARKer<x>:X:FREQuency	Sets or queries the marker frequency.
CALCulate:SGRam:MARKer<x>:X[:TIME]	Sets or queries the marker time.
CALCulate:SGRam:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:SPECTrum subgroup	Spectrum measurement
CALCulate:SPECTrum:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
CALCulate:SPECTrum:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:SPECTrum:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.

Table 2-12: Calculate commands (cont.)

Header	Description
CALCulate:SPECtrum:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:SPECtrum:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:SPECtrum:MARKer<x>[:SET]:CENTer	Sets the center frequency to the marker frequency.
CALCulate:SPECtrum:MARKer<x>:TRACe	Sets or queries the trace on which the marker is placed.
CALCulate:SPECtrum:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:SPECtrum:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:SPURious subgroup	Spurious measurement
CALCulate:SPURious:MARKer<x>:DELta:X?	Returns the delta marker frequency for the selected marker.
CALCulate:SPURious:MARKer<x>:DELta:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:SPURious:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:SPURious:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:SPURious:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:SPURious:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:SPURious:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:SPURious:MARKer<x>[:SET]:CENTer	Sets the center frequency to the marker frequency.
CALCulate:SPURious:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:SPURious:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:TDIagram subgroup (Option 21 only)	Trellis diagram
CALCulate:TDIagram:MARKer<x>:DELta:X[:TIME]?	Returns the delta marker time for the selected marker.
CALCulate:TDIagram:MARKer<x>:DELta:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:TDIagram:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:TDIagram:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:TDIagram:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:TDIagram:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:TDIagram:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:TDIagram:MARKer<x>:X[:TIME]	Sets or queries the horizontal position (time) of the marker.
CALCulate:TDIagram:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.
CALCulate:TOVerview subgroup	Time overview
CALCulate:TOVerview:MARKer<x>:DELta:X?	Returns the delta marker time for the selected marker.
CALCulate:TOVerview:MARKer<x>:DELta:Y?	Returns the delta marker amplitude for the selected marker.
CALCulate:TOVerview:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
CALCulate:TOVerview:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
CALCulate:TOVerview:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
CALCulate:TOVerview:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
CALCulate:TOVerview:MARKer<x>:X	Sets or queries the horizontal position of the marker.
CALCulate:TOVerview:MARKer<x>:Y?	Queries the marker amplitude of the selected marker.

Marker Mnemonics

Up to five markers can be used. In commands, these are named MARKer<x>, where <x> can be 0, 1, 2, 3, or 4 as shown in the following table.

Table 2-13: Marker mnemonics

Mnemonic	Description
MARKer0	Reference marker (MR)
MARKer1	Marker 1 (M1)
MARKer2	Marker 2 (M2)
MARKer3	Marker 3 (M3)
MARKer4	Marker 4 (M4)

NOTE. *If you omit the numeric suffix, the marker control defaults to Marker 1.*

Before operating the marker, you have to enable it using the CALCulate basic commands.

If you attempt to use a marker other than above in a CALCulate command, the suffix error (error code -130) will occur.

Calibration Commands

Use the CALibration commands to control the external correction.

Table 2-14: Calibration commands

Header	Description
CALibration:ABORT	Aborts any actions related to the alignments in progress.
CALibration:AUTO	Sets or queries whether or not to run alignments automatically.
CALibration:CORRection:EXTeRnal:EDIT<x>:LABel	Sets or queries the name of the external loss table.
CALibration:CORRection:EXTeRnal:EDIT<x>:NEw	Creates a new external loss table.
CALibration:CORRection:EXTeRnal:EDIT<x>:STATe	Sets or queries whether to enable or disable the external loss table.
CALibration:CORRection:EXTeRnal:GAIN[:MAGNitude]	Sets or queries the external gain value.
CALibration:CORRection:EXTeRnal:GAIN:STATe	Sets or queries whether to enable or disable the external gain value.
CALibration:CORRection:EXTeRnal:PROBe:CONNeCt?	Queries whether the external probe is connected to the analyzer or not.
CALibration:CORRection:EXTeRnal:PROBe[:MAGNitude]?	Queries the external probe attenuation.
CALibration:CORRection:EXTeRnal:PROBe:STATe	Determines whether to correct data for the external probe attenuation.
CALibration:CORRection:EXTeRnal:TYPE	Selects data type to use when applying the external loss table.

Display Commands

Use the DISPLAY commands to control the display of measurement waveforms and results on the screen.

Table 2-15: Display commands

Header	Description
DISPlay basic command subgroup	General window control
DISPlay:WINDow:ACTive:MEASurement?	Queries the active measurement views.
DISPlay:WINDow:COLor:SCHEME	Sets or queries the color scheme for traces and background.
DISPlay:WINDow:OPTimized:MEASurement?	Queries the measurement views that are optimized.
DISPlay:ACPower subgroup	Channel power and ACPR measurement
DISPlay:ACPower:MARKer:SHOW:STATe	Determines whether to show the readout for the selected marker.
DISPlay:ACPower:PLEVel:SHOW:STATe	Determines whether to show the power levels.
DISPlay:ACPower:RESet:SCALE	Resets the horizontal and vertical scale to the default values.
DISPlay:ACPower:WINDow:TRACe:GRATICule:GRID:STATe	Determines whether to show the graticule grid on screen.
DISPlay:ACPower:X[:SCALE]	Sets or queries the horizontal range.
DISPlay:ACPower:X[:SCALE]:AUTO	Rescales the horizontal axis automatically.
DISPlay:ACPower:X[:SCALE]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:ACPower:Y[:SCALE]	Sets or queries the vertical range.
DISPlay:ACPower:Y[:SCALE]:AUTO	Rescales the vertical axis automatically.
DISPlay:ACPower:Y[:SCALE]:OFFSet	Sets or queries the vertical offset.
DISPlay:ADEMod subgroup (Option 21 only)	General purpose analog demodulation measurements
DISPlay:ADEMod:MEASview:DELete	Deletes the measurement view.
DISPlay:ADEMod:MEASview:NEW	Displays a new measurement view.
DISPlay:ADEMod:MEASview:SELect	Sets or queries the measurement view.
DISPlay:{AM FM PM} subgroup (Option 21 only)	AM/FM/PM measurement
DISPlay:{AM FM PM}:MARKer:SHOW:STATe	Determines whether to show the readout for the selected marker.
DISPlay:{AM FM PM}:WINDow:TRACe:GRATICule:GRID:STATe	Determines whether to show the graticule grid on screen.
DISPlay:{AM FM PM}:X:RScale	Rescales the horizontal axis automatically.
DISPlay:{AM FM PM}:X[:SCALE]:AUTO	Sets the horizontal scale automatically.
DISPlay:{AM FM PM}:X[:SCALE]:FULL	Sets or queries the horizontal scale.
DISPlay:{AM FM PM}:X[:SCALE]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:{AM FM PM}:Y:RScale	Rescales the vertical axis automatically.
DISPlay:{AM FM PM}:Y[:SCALE]	Sets or queries the vertical scale.
DISPlay:{AM FM PM}:Y[:SCALE]:OFFSet	Sets or queries the vertical offset.
DISPlay:AVTime subgroup	Amplitude versus Time measurement

Table 2-15: Display commands (cont.)

Header	Description
DISPlay:AVTime:LEGenD:STATe	Shows or hides the trace legend in the amplitude versus time view.
DISPlay:AVTime:MARKer:SHOW:STATe	Determines whether to show the readout for the selected marker.
DISPlay:AVTime:RESet	Resets the horizontal and vertical scale to the default values.
DISPlay:AVTime:TRIGger:LEVel:STATe	Determines whether to show the power trigger level line on screen.
DISPlay:AVTime:WINDow:TRACe:GRATICule:GRID:STATe	Determines whether to show the graticule grid on screen.
DISPlay:AVTime:X:RSCale	Rescales the horizontal axis automatically.
DISPlay:AVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
DISPlay:AVTime:X[:SCALe]:AUTO:STATe	Determines whether to set the horizontal scale automatically or manually.
DISPlay:AVTime:X[:SCALe]:FULL	Sets or queries the horizontal scale.
DISPlay:AVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
DISPlay:AVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
DISPlay:AVTime:X[:SCALe]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:AVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
DISPlay:AVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
DISPlay:AVTime:Y:RSCale	Rescales the vertical axis automatically.
DISPlay:AVTime:Y[:SCALe]:FULL	Sets or queries the vertical scale.
DISPlay:AVTime:Y[:SCALe]:OFFSet	Sets or queries the vertical offset.
DISPlay:CCDF subgroup	CCDF measurement
DISPlay:CCDF:LEGenD:STATe	Sets or queries whether to show or hide the trace legend in the CCDF view.
DISPlay:CCDF:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries whether to show or hide the graticule grid on the screen.
DISPlay:CONSte subgroup (Option 21 only)	Constellation measurement
DISPlay:CONSte:MPHase	Sets or queries the phase multiplication constant for a CPM signal.
DISPlay:CONSte:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries whether to show the graticule grid on the screen.
DISPlay:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
DISPlay:DDEMod:MEASview:DELeTe	Deletes the measurement view.
DISPlay:DDEMod:MEASview:NEw	Displays a new measurement view.
DISPlay:DDEMod:MEASview:SELeCt	Sets or queries the measurement view.
DISPlay:DDEMod:RADix	Sets or queries the base of symbols.
DISPlay:DDEMod:X[:SCALe]	Sets or queries the horizontal scale.
DISPlay:DDEMod:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
DISPlay:DDEMod:X[:SCALe]:AUTO:STATe	Determines whether to set the horizontal scale automatically or manually.
DISPlay:DDEMod:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
DISPlay:DDEMod:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
DISPlay:DDEMod:X[:SCALe]:OFFSet	Sets or queries the minimum horizontal value (left edge).

Table 2-15: Display commands (cont.)

Header	Description
<code>DISPlay:DDEMod:X[:SCALe]:OFFSet:MAXimum?</code>	Queries the upper limit of the horizontal offset setting range.
<code>DISPlay:DDEMod:X[:SCALe]:OFFSet:MINimum?</code>	Queries the lower limit of the horizontal offset setting range.
<code>DISPlay:DDEMod:X[:SCALe]:RESet</code>	Presets the horizontal scale to the default value.
DISPlay:DIAGram subgroup (Option 21 only)	Eye/Trellis diagram
<code>DISPlay:DIAGram:X[:SCALe]</code>	Sets or queries the horizontal range.
<code>DISPlay:DIAGram:X[:SCALe]:RESet</code>	Presets the horizontal scale to the default value.
DISPlay:DIQVtime subgroup (Option 21 only)	Demodulated I&Q versus Time measurement
<code>DISPlay:DIQVtime:WINDow:TRACe:GRATicule:GRID:STATe</code>	Sets or queries whether to show the graticule grid on the screen.
<code>DISPlay:DIQVtime:Y[:SCALe]</code>	Sets or queries the vertical scale.
<code>DISPlay:DIQVtime:Y[:SCALe]:AUTO</code>	Sets the vertical scale automatically.
<code>DISPlay:DIQVtime:Y[:SCALe]:OFFSet</code>	Sets or queries the vertical offset (center point of the vertical axis).
DISPlay:DPSA subgroup	DPX spectrum measurement
<code>DISPlay:DPSA:LEGend:STATe</code>	Show or hide the trace legend on the display.
<code>DISPlay:DPSA:WINDow:TRACe:GRATicule:GRID:STATe</code>	Show or hide the graticule grid on the screen.
<code>DISPlay:DPSA:Y[:SCALe]:PDIVision</code>	Sets or queries the vertical scale (per division).
DISPlay:EDIagram subgroup (Option 21 only)	Eye diagram
<code>DISPlay:EDIagram:WINDow:TRACe:GRATicule:GRID:STATe</code>	Sets or queries whether to show the graticule grid on the screen.
<code>DISPlay:EDIagram:Y[:SCALe]</code>	Sets or queries the vertical scale.
<code>DISPlay:EDIagram:Y[:SCALe]:AUTO</code>	Sets the vertical scale automatically.
<code>DISPlay:EDIagram:Y[:SCALe]:OFFSet</code>	Sets or queries the vertical offset (center point of the vertical axis).
DISPlay:EVM subgroup (Option 21 only)	EVM versus Time measurement
<code>DISPlay:EVM:WINDow:TRACe:GRATicule:GRID:STATe</code>	Sets or queries the graticule grid view state for the EVM view.
<code>DISPlay:EVM:Y[:SCALe]</code>	Sets or queries the vertical scale.
<code>DISPlay:EVM:Y[:SCALe]:AUTO</code>	Sets the vertical scale automatically.
<code>DISPlay:EVM:Y[:SCALe]:OFFSet</code>	Sets or queries the minimum vertical value (bottom edge).
DISPlay:FDVTime subgroup (Option 21 only)	Frequency deviation versus Time measurement
<code>DISPlay:FDVTime:WINDow:TRACe:GRATicule:GRID:STATe</code>	Sets or queries whether to show the graticule grid on the Frequency deviation versus Time view.
<code>DISPlay:FDVTime:Y[:SCALe]</code>	Sets or queries the vertical range of the Frequency deviation versus Time graph.
<code>DISPlay:FDVTime:Y[:SCALe]:AUTO</code>	Sets the vertical scale automatically.
<code>DISPlay:FDVTime:Y[:SCALe]:OFFSet</code>	Sets or queries the vertical offset (center point of the vertical axis).
DISPlay:FVTime subgroup	Frequency versus Time measurement

Table 2-15: Display commands (cont.)

Header	Description
DISPlay:FVTime:WINDow:TRACe:GRATICule:GRID:STATE	Sets or queries whether to show the graticule grid on the Frequency versus Time view.
DISPlay:FVTime:X[:SCALe]	Sets or queries the horizontal scale.
DISPlay:FVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
DISPlay:FVTime:X[:SCALe]:AUTO:STATE	Determines whether to set the horizontal scale automatically or manually.
DISPlay:FVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
DISPlay:FVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
DISPlay:FVTime:X[:SCALe]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:FVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
DISPlay:FVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
DISPlay:FVTime:Y[:SCALe]	Sets or queries the vertical scale.
DISPlay:FVTime:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
DISPlay:FVTime:Y[:SCALe]:OFFSet	Sets or queries the vertical offset.
DISPlay:GENeral subgroup	General signal viewing
DISPlay:GENeral:MEASview:DELeTe	Deletes the measurement view.
DISPlay:GENeral:MEASview:NEW	Displays a new measurement view.
DISPlay:GENeral:MEASview:SELeCt	Sets or queries the measurement view.
DISPlay:GPRF subgroup	General purpose RF measurements
DISPlay:GPRF:MEASview:DELeTe	Deletes the measurement view.
DISPlay:GPRF:MEASview:NEW	Displays a new measurement view.
DISPlay:GPRF:MEASview:SELeCt	Sets or queries the measurement view.
DISPlay:IQVTime subgroup	RF I&Q versus Time measurement
DISPlay:IQVTime:WINDow:TRACe:GRATICule:GRID:STATE	Sets or queries whether to show the graticule grid on the screen.
DISPlay:IQVTime:X[:SCALe]	Sets or queries the horizontal scale.
DISPlay:IQVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
DISPlay:IQVTime:X[:SCALe]:AUTO:STATE	Determines whether to set the horizontal scale automatically or manually.
DISPlay:IQVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
DISPlay:IQVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
DISPlay:IQVTime:X[:SCALe]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
DISPlay:IQVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
DISPlay:IQVTime:Y[:SCALe]	Sets or queries the vertical scale.
DISPlay:IQVTime:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
DISPlay:IQVTime:Y[:SCALe]:OFFSet	Sets or queries the vertical offset.
DISPlay:IQVTime:Y[:SCALe]:RESCale	Rescales the vertical scale.
DISPlay:MCPR subgroup	MCPR measurement

Table 2-15: Display commands (cont.)

Header	Description
DISPlay:MCPower:MARKer:SHOW:STATe	Determines whether to show the readout for the selected marker.
DISPlay:MCPower:PLEvel:SHOW:STATe	Determines whether to show the power levels.
DISPlay:MCPower:RESet:SCALE	Resets the horizontal and vertical scale to the default values.
DISPlay:MCPower:WINDow:TRACe:GRATICule:GRID:STATe	Determines whether to show the graticule grid on screen.
DISPlay:MCPower:X[:SCALE]	Sets or queries the horizontal range.
DISPlay:MCPower:X[:SCALE]:AUTO	Rescales the horizontal axis automatically.
DISPlay:MCPower:X[:SCALE]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:MCPower:Y[:SCALE]	Sets or queries the vertical range.
DISPlay:MCPower:Y[:SCALE]:AUTO	Rescales the vertical axis automatically.
DISPlay:MCPower:Y[:SCALE]:OFFSet	Sets or queries the vertical offset.
DISPlay:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
DISPlay:MERRor:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries the graticule grid view state for the Magnitude error versus Time view.
DISPlay:MERRor:Y[:SCALE]	Sets or queries the vertical scale.
DISPlay:MERRor:Y[:SCALE]:AUTO	Sets the vertical scale automatically.
DISPlay:MERRor:Y[:SCALE]:OFFSet	Sets or queries the minimum vertical value (bottom edge).
DISPlay:OBWidth subgroup	Occupied Bandwidth measurement
DISPlay:OBWidth:MARKer:SHOW:STATe	Determines whether to show the readout for the selected marker.
DISPlay:OBWidth:RESet:SCALE	Resets the horizontal and vertical scale to the default values.
DISPlay:OBWidth:SELected:BANDwidth	Sets or queries the bandwidth (OBW or x dB BW) to measure.
DISPlay:OBWidth:WINDow:TRACe:GRATICule:GRID:STATe	Determines whether to show the graticule grid on screen.
DISPlay:OBWidth:X[:SCALE]	Sets or queries the horizontal range.
DISPlay:OBWidth:X[:SCALE]:AUTO	Rescales the horizontal axis automatically.
DISPlay:OBWidth:X[:SCALE]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:OBWidth:Y[:SCALE]	Sets or queries the vertical range.
DISPlay:OBWidth:Y[:SCALE]:AUTO	Rescales the vertical axis automatically.
DISPlay:OBWidth:Y[:SCALE]:OFFSet	Sets or queries the vertical offset.
DISPlay:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
DISPlay:PERRor:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries the graticule grid view state for the Phase error versus Time view.
DISPlay:PERRor:Y[:SCALE]	Sets or queries the vertical scale.
DISPlay:PERRor:Y[:SCALE]:AUTO	Sets the vertical scale automatically.
DISPlay:PERRor:Y[:SCALE]:OFFSet	Sets or queries the minimum vertical value (bottom edge).
DISPlay:PHVTime subgroup	Phase versus Time measurement
DISPlay:PHVTime:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries whether to show the graticule grid on the screen.

Table 2-15: Display commands (cont.)

Header	Description
DISPlay:PHVTime:X[:SCALe]	Sets or queries the horizontal scale.
DISPlay:PHVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
DISPlay:PHVTime:X[:SCALe]:AUTO:STATe	Determines whether to set the horizontal scale automatically or manually.
DISPlay:PHVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
DISPlay:PHVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
DISPlay:PHVTime:X[:SCALe]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:PHVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
DISPlay:PHVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
DISPlay:PHVTime:Y[:SCALe]	Sets or queries the vertical scale.
DISPlay:PHVTime:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
DISPlay:PHVTime:Y[:SCALe]:AXIS	Sets or queries the vertical axis representation.
DISPlay:PHVTime:Y[:SCALe]:AXIS:REFerence	Sets or queries the reference time for phase.
DISPlay:PHVTime:Y[:SCALe]:OFFSet	Sets or queries the vertical offset.
DISPlay:PHVTime:Y[:SCALe]:RESCale	Rescales the vertical scale.
DISPlay:PNOise subgroup (Option 11 only)	Phase noise measurements
DISPlay:PNOise:LEGend:STATe	Sets or queries showing the trace legend on the display.
DISPlay:PNOise:MARKer:SHOW:STATe	Determines whether to show the readout for the selected marker.
DISPlay:PNOise:RESet:SCALe	Resets the horizontal and vertical scale to the default values.
DISPlay:PNOise:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries whether to show the graticule grid on the screen.
DISPlay:PNOise:X[:SCALe]:AUTO	Rescales the horizontal axis automatically.
DISPlay:PNOise:X[:SCALe]:START	Sets or queries the start frequency of the graph.
DISPlay:PNOise:X[:SCALe]:STOP	Sets or queries the stop frequency of the graph.
DISPlay:PNOise:Y[:SCALe]	Sets or queries the vertical scale.
DISPlay:PNOise:Y[:SCALe]:AUTO	Rescales the vertical axis automatically.
DISPlay:PNOise:Y[:SCALe]:OFFSet	Sets or queries the vertical offset.
DISPlay:PNOise:Y[:SCALe]:PDIvision	Sets or queries the vertical scale (per division).
DISPlay:PULSe subgroup (Option 20 only)	Pulsed RF measurements
DISPlay:PULSe:MEASview:DELeTe	Deletes the measurement view.
DISPlay:PULSe:MEASview:NEw	Displays a new measurement view.
DISPlay:PULSe:MEASview:SELeCt	Sets or queries the measurement view.
DISPlay:PULSe:RESult:ATX	Sets or queries whether to show the average transmitted power result.
DISPlay:PULSe:RESult:AVERage	Sets or queries whether to show the average on power result.
DISPlay:PULSe:RESult:DRODb	Sets or queries whether to show the droop in the results table.
DISPlay:PULSe:RESult:DROOp	Sets or queries showing the droop measurement result in the pulse table
DISPlay:PULSe:RESult:DUTPct	Sets or queries whether to show the duty factor (%) result.
DISPlay:PULSe:RESult:DUTRatio	Sets or queries whether to show the duty factor (ratio) result.

Table 2-15: Display commands (cont.)

Header	Description
<code>DISPlay:PULSe:RESult:FALL</code>	Sets or queries whether to show the fall time in the results table.
<code>DISPlay:PULSe:RESult:FRDeviation</code>	Sets or queries whether to show the frequency deviation result.
<code>DISPlay:PULSe:RESult:IRAmplitude</code>	Sets or queries showing the Impulse Response Amplitude measurement result in the pulse table.
<code>DISPlay:PULSe:RESult:IRTime</code>	Sets or queries showing the Impulse Response Time measurement result in the pulse table.
<code>DISPlay:PULSe:RESult:MFRerror</code>	Sets or queries whether to show the maximum frequency error result.
<code>DISPlay:PULSe:RESult:MPHerror</code>	Sets or queries whether to show the maximum phase error result.
<code>DISPlay:PULSe:RESult:OVEDb</code>	Sets or queries whether to show the Overshoot measurement result in dB in the pulse table.
<code>DISPlay:PULSe:RESult:OVERshoot</code>	Sets or queries whether to show the Overshoot measurement result in the pulse table.
<code>DISPlay:PULSe:RESult:PHDeviation</code>	Sets or queries whether to show the phase deviation result.
<code>DISPlay:PULSe:RESult:PPFrequency</code>	Sets or queries whether to show the pulse-pulse frequency result.
<code>DISPlay:PULSe:RESult:PPOWER</code>	Sets or queries whether to show the peak power in the results table.
<code>DISPlay:PULSe:RESult:PPPHas</code>	Sets or queries whether to show the pulse-pulse carrier phase result.
<code>DISPlay:PULSe:RESult:RINTerval</code>	Sets or queries whether to show the repetition interval result.
<code>DISPlay:PULSe:RESult:RIPDb</code>	Sets or queries showing the ripple measurement result in dB in the pulse table.
<code>DISPlay:PULSe:RESult:RIPple</code>	Sets or queries showing the ripple measurement result in the pulse table.
<code>DISPlay:PULSe:RESult:RISE</code>	Sets or queries whether to show the rise time in the results table.
<code>DISPlay:PULSe:RESult:RMSFreqerror</code>	Sets or queries whether to show the RMS frequency error result.
<code>DISPlay:PULSe:RESult:RMSPherror</code>	Sets or queries whether to show the RMS phase error result.
<code>DISPlay:PULSe:RESult:RRATE</code>	Sets or queries whether to show the repetition rate result.
<code>DISPlay:PULSe:RESult:TIME</code>	Sets or queries whether to show the time in the results table.
<code>DISPlay:PULSe:RESult:WIDTH</code>	Sets or queries whether to show the pulse width in the results table.
<code>DISPlay:PULSe:SElect:NUMBER</code>	Sets or queries the pulse to measure.
<code>DISPlay:PULSe:SElect:RESult</code>	Sets or queries which result is shown in the trace and statistics views.
<code>DISPlay:PULSe:STATistics:MARKer:SHOW:STATe</code>	Sets or queries whether to show the marker readout in the graph.
<code>DISPlay:PULSe:STATistics:PLOT</code>	Sets or queries how to show the statistics graph.
<code>DISPlay:PULSe:STATistics:WINDow:TRACe:GRATICule:GRID:STATe</code>	Sets or queries whether to show the graticule grid in the statistics view.
<code>DISPlay:PULSe:STATistics:X:RSCale</code>	Rescales the horizontal axis of the statistics graph.
<code>DISPlay:PULSe:STATistics:X[:SCALE]:NUMBER</code>	Sets or queries the horizontal scale (the number of pulses per division).
<code>DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet</code>	Sets or queries the minimum horizontal value in the statistics view.
<code>DISPlay:PULSe:STATistics:Y:RSCale</code>	Rescales the vertical axis of the statistics graph.
<code>DISPlay:PULSe:STATistics:Y[:SCALE]:FULL</code>	Sets or queries the vertical full-scale in the statistics view.
<code>DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet</code>	Sets or queries the vertical offset in the statistics view.

Table 2-15: Display commands (cont.)

Header	Description
DISPlay:PULSe:STATistics:Y[:SCALE]:STOP?	Queries the minimum vertical value in the statistics view.
DISPlay:PULSe:TRACe:MARKer:SHOW:STATe	Sets or queries whether to show the marker readout in the trace view.
DISPlay:PULSe:TRACe:POINt:SHOW	Sets or queries whether to show the measurement points and lines.
DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe	Sets or queries whether to show the graticule grid in the trace view.
DISPlay:PULSe:TRACe:X:RSCale	Rescales the horizontal axis of the pulse trace view.
DISPlay:PULSe:TRACe:X[:SCALE]	Sets or queries the horizontal full scale in the pulse trace view.
DISPlay:PULSe:TRACe:X[:SCALE]:FULL	Sets or queries the full-scale reference for the horizontal rescale.
DISPlay:PULSe:TRACe:X[:SCALE]:OFFSet	Sets or queries the minimum horizontal value in the pulse trace view.
DISPlay:PULSe:TRACe:X[:SCALE]:PDIVision	Sets or queries the horizontal full scale in the pulse trace view.
DISPlay:PULSe:TRACe:Y:RSCale	Rescales the vertical axis of the pulse trace view.
DISPlay:PULSe:TRACe:Y[:SCALE]:FULL	Sets or queries the vertical full scale in the pulse trace view.
DISPlay:PULSe:TRACe:Y[:SCALE]:OFFSet	Sets or queries the vertical offset in the pulse trace view.
DISPlay:PULSe:TRACe:Y[:SCALE]:STOP?	Queries the minimum vertical value in the pulse trace view.
DISPlay:SGRam subgroup	Spectrogram measurement
DISPlay:SGRam:FREQuency:AUTO	Rescales the horizontal (frequency) axis automatically.
DISPlay:SGRam:FREQuency:OFFSet	Sets or queries the horizontal (frequency) offset.
DISPlay:SGRam:FREQuency:SCAle	Sets or queries the horizontal (frequency) range.
DISPlay:SGRam:TIME:AUTO	Rescales the vertical axis automatically.
DISPlay:SGRam:TIME:OFFSet	Sets or queries the vertical axis (time) offset (bottom line number).
DISPlay:SGRam:TIME:OVERlap	Determines whether or not to allow overlap between adjacent FFT frames.
DISPlay:SGRam:TIME:SCAle	Sets or queries the vertical scale (the amount of time in each line).
DISPlay:SPECtrum subgroup	Spectrum measurement
DISPlay:SPECtrum:FREQuency:AUTO	Rescales the horizontal (frequency) axis automatically.
DISPlay:SPECtrum:FREQuency:OFFSet	Sets or queries the horizontal (frequency) offset.
DISPlay:SPECtrum:FREQuency[:SCALE]	Sets or queries the horizontal (frequency) range.
DISPlay:SPECtrum:MARKer:NOISe:MODE	Sets or queries whether to enable the marker noise mode.
DISPlay:SPECtrum:SCALE:LOG:STATe	Sets or queries whether to set the horizontal axis logarithmic.
DISPlay:SPECtrum:WINDow:TRACe:GRATicule:GRID:STATe	Sets or queries whether to show the graticule grid.
DISPlay:SPECtrum:WINDow:TRACe:LEGend:STATe	Show or hide the trace legend in the Spectrum view.
DISPlay:SPECtrum:X:LABel	Sets or queries the labels for the horizontal axis.
DISPlay:SPECtrum:Y[:SCALE]	Sets or queries the vertical range.
DISPlay:SPECtrum:Y[:SCALE]:AUTO	Rescales the vertical axis automatically.
DISPlay:SPECtrum:Y[:SCALE]:OFFSet	Sets or queries the vertical offset.
DISPlay:SPECtrum:Y[:SCALE]:PDIVision	Sets or queries the vertical scale (per division).
DISPlay:SPECtrum:Y[:SCALE]:RESet	Resets the vertical scale to the default values.

Table 2-15: Display commands (cont.)

Header	Description
DISPlay:SPURious subgroup	Spurious measurement
DISPlay:SPURious:MARKer:SHOW:STATe	Sets or queries whether to show the readout for the selected marker.
DISPlay:SPURious:RESet:SCALe	Resets the horizontal and vertical scale to the default values.
DISPlay:SPURious:SCALe:LOG:STATe	Sets or queries whether to set the horizontal axis logarithmic.
DISPlay:SPURious:SElect:NUMBER	Sets or queries the spurious number.
DISPlay:SPURious:SHOW:LIMit	Sets or queries how to display the limits.
DISPlay:SPURious:WINDow:TRACe:GRATICule:GRID:STATe	Determines whether to show the graticule grid on screen.
DISPlay:SPURious:X[:SCALe]:AUTO	Rescales the horizontal axis automatically.
DISPlay:SPURious:X[:SCALe]:START	Sets or queries the minimum horizontal value of the spectrum graph.
DISPlay:SPURious:X[:SCALe]:STOP	Sets or queries the maximum horizontal value of the spectrum graph.
DISPlay:SPURious:Y[:SCALe]	Sets or queries the vertical range of the spectrum graph.
DISPlay:SPURious:Y[:SCALe]:AUTO	Rescales the vertical axis automatically.
DISPlay:SPURious:Y[:SCALe]:OFFSet	Sets or queries the vertical offset of the spectrum graph.
DISPlay:TDIagram subgroup (Option 21 only)	Trellis diagram
DISPlay:TDIagram:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries whether to show the graticule grid on the screen.
DISPlay:TDIagram:Y[:SCALe]	Sets or queries the vertical scale.
DISPlay:TDIagram:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
DISPlay:TDIagram:Y[:SCALe]:OFFSet	Sets or queries the vertical offset (center point of the vertical axis).
DISPlay:TOVerview subgroup	Time overview
DISPlay:TOVerview:WINDow:TRACe:GRATICule:GRID:STATe	Sets or queries whether to show the graticule grid in the time overview.
DISPlay:TOVerview:X[:SCALe]	Sets or queries the horizontal scale.
DISPlay:TOVerview:X[:SCALe]:AUTO	Sets the horizontal scale and offset automatically.
DISPlay:TOVerview:X[:SCALe]:OFFSet	Sets or queries the minimum horizontal value (left edge).
DISPlay:TOVerview:Y[:SCALe]	Sets or queries the vertical scale.
DISPlay:TOVerview:Y[:SCALe]:AUTO	Sets the vertical scale and offset automatically.
DISPlay:TOVerview:Y[:SCALe]:OFFSet	Sets or queries the vertical offset.
DISPlay:TOVerview:Y[:SCALe]:RESCale	Rescales the vertical scale.
DISPlay:WINDow subgroup	Window display
DISPlay:WINDow:ACTive:MEASurement?	Queries the active measurement views
DISPlay:WINDow:COLor:SCHEME	Sets or queries the color scheme for displaying traces and background on the screen.
DISPlay:WINDow:OPTimized:MEASurement?	Queries the measurement views that are optimized.

Fetch Commands

The FETCh commands retrieve the measurements from the data taken by the latest INITiate command.

To perform a FETCh operation on fresh data, use the READ commands, which acquire a new input signal and fetch the measurement results from that data.

Table 2-16: Fetch commands

Header	Description
FETCh basic command subgroup	General fetch control
FETCh:RFIN:IQ?	Returns time-domain IQ data for a specific acquisition data record.
FETCh:RFIN:IQ:HEADer?	Returns the header information for a specific acquisition data record.
FETCh:RFIN:IQ:SCALe?	Returns the scaling factor contained in the .tiq file header.
FETCh:RFIN:RECOrd:IDS?	Returns the beginning and end ID numbers of acquisition data.
FETCh:ACPower subgroup	Channel power and ACPR measurement
FETCh:ACPower?	Returns the ACPR measurement results.
FETCh:ACPower:CHANnel:POWer?	Returns the average power of the main channel.
FETCh:ACPower:SPECTrum?	Returns spectrum trace data of the ACPR measurement.
FETCh:{AM FM PM} subgroup (Option 21 only)	AM/FM/PM measurement
FETCh:{AM FM PM}?	Returns the trace data.
FETCh:AM:AMINdex?	FIRST Returns the modulation depth.
FETCh:AM:AMNegative?	Returns the negative peak modulation factor (-AM).
FETCh:AM:AMPositive?	Returns the positive peak modulation factor (+AM).
FETCh:AM:RESult?	Returns the AM measurement results.
FETCh:{FM PM}:FERRor?	Returns the frequency error in the Frequency or Phase modulation measurement.
FETCh:FM:PHALf?	Returns the half peak-peak frequency deviation (Pk-Pk/2).
FETCh:FM:PNEGative?	Returns the negative peak frequency deviation (-Pk).
FETCh:FM:PPOSitive?	Returns the positive peak frequency deviation (+Pk).
FETCh:FM:PTPeak?	Returns the peak-peak frequency deviation (Pk-Pk).
FETCh:FM:RESult?	Returns the FM measurement results.
FETCh:FM:RMS?	Returns the RMS frequency deviation.
FETCh:PM:PNEGative?	Returns the negative peak phase deviation (-Pk).
FETCh:PM:PPOSitive?	Returns the positive peak phase deviation (+Pk).
FETCh:PM:PTPeak?	Returns the peak-peak phase deviation (Pk-Pk).
FETCh:PM:RESult?	Returns the PM measurement results.
FETCh:PM:RMS?	Returns the RMS phase deviation.
FETCh:AVTime subgroup	Amplitude versus Time measurement
FETCh:AVTime:AVERage?	Returns the RMS value.

Table 2-16: Fetch commands (cont.)

Header	Description
FETCh:AVTime:{FIRST SECOnd THIRd FOURth}?	Returns the trace data.
FETCh:AVTime:MAXimum?	Returns the maximum value.
FETCh:AVTime:MAXLocation?	Returns the time at the maximum.
FETCh:AVTime:MINimum?	Returns the minimum value.
FETCh:AVTime:MINLocation?	Returns the time at the minimum.
FETCh:AVTime:RESult?	Returns the measurement results.
FETCh:CCDF subgroup	CCDF measurement
FETCh:CCDF?	Returns the CCDF measurement results.
FETCh:CCDF:{FIRST SECOnd THIRd}:X?	Returns the horizontal values of the specified trace.
FETCh:CCDF:{FIRST SECOnd THIRd}:XY?	Returns the horizontal and vertical value pairs of the specified trace.
FETCh:CCDF:{FIRST SECOnd THIRd}:Y?	Returns the vertical values of the specified trace.
FETCh:CONSte subgroup (Option 21 only)	Constellation measurement
FETCh:CONSte:FERRor?	Returns the frequency error in Hz.
FETCh:CONSte:RESults?	Returns the constellation measurement results.
FETCh:CONSte:TRACe?	Returns the constellation trace data.
FETCh:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
FETCh:DDEMod:STABle?	Returns the symbol table data.
FETCh:DDEMod:SYNCh:WORD:LENGth?	Returns the length of the synch word in the symbol table.
FETCh:DDEMod:SYNCh:WORD:POSition?	Returns the position of the synch word in the symbol table.
FETCh:DIQVtime subgroup (Option 21 only)	Demodulated I&Q versus Time measurement
FETCh:DIQVtime:FERRor?	Returns the frequency error.
FETCh:DIQVtime:I?	Returns the I versus Time trace data.
FETCh:DIQVtime:Q?	Returns the Q versus Time trace data.
FETCh:DPSA subgroup	DPX spectrum measurement
FETCh:DPSA:RESults:TRACe<x>?	Returns waveform data in the DPX spectrum measurement.
FETCh:DPSA:TRACe:AVERAge?	Returns waveform data of the average trace in the DPX spectrum measurement.
FETCh:DPSA:TRACe:BITMap?	Returns trace waveform data of the bitmap trace.
FETCh:DPSA:TRACe:MATH?	Returns waveform data of the math trace.
FETCh:DPSA:TRACe:MAXimum?	Returns waveform data of the maximum trace.
FETCh:DPSA:TRACe:MINimum?	Returns waveform data of the minimum trace.
FETCh:EDlagram subgroup (Option 21 only)	Eye diagram
FETCh:EDlagram:FDEVIation?	Returns the frequency deviation versus Time trace data.
FETCh:EDlagram:FERRor?	Returns the frequency error.
FETCh:EDlagram:I?	Returns the I versus Time trace data.
FETCh:EDlagram:Q?	Returns the Q versus Time trace data.
FETCh:EVM subgroup (Option 21 only)	EVM versus Time measurement

Table 2-16: Fetch commands (cont.)

Header	Description
FETCh:EVM:FERRor?	Returns the frequency error.
FETCh:EVM:PEAK?	Returns the peak value.
FETCh:EVM:PINDex?	Returns the time at the EVM peak.
FETCh:EVM:RMS?	Returns the RMS value.
FETCh:EVM:TRACe?	Returns the EVM versus Time trace data.
FETCh:FDVTime subgroup (Option 21 only)	Frequency deviation versus Time measurement
FETCh:FDVTime:FERRor?	Returns the frequency error in the Frequency deviation versus Time measurement.
FETCh:FDVTime:TRACe?	Returns the Frequency deviation versus Time trace data.
FETCh:FVTime subgroup	Frequency versus Time measurement
FETCh:FVTime?	Returns the Frequency versus Time trace data.
FETCh:FVTime:MAXimum?	Returns the maximum value.
FETCh:FVTime:MAXLocation?	Returns the time at which the frequency drift is maximum.
FETCh:FVTime:MINimum?	Returns the minimum value.
FETCh:FVTime:MINLocation?	Returns the time at which the frequency drift is minimum.
FETCh:FVTime:RESult?	Returns the measurement results.
FETCh:IQVTime subgroup	RF I&Q versus Time measurement
FETCh:IQVTime:I?	Returns the I versus Time trace data.
FETCh:IQVTime:MAXimum?	Returns the maximum value.
FETCh:IQVTime:MAXLocation?	Returns the time at which the I or Q level is maximum.
FETCh:IQVTime:MINimum?	Returns the minimum value.
FETCh:IQVTime:MINLocation?	Returns the time at which the I or Q level is minimum.
FETCh:IQVTime:Q?	Returns the Q versus Time trace data.
FETCh:IQVTime:RESult?	Returns the measurement results.
FETCh:MCPower subgroup	MCPR measurement
FETCh:MCPower:ADJacent:CHANnels?	Returns the power of adjacent channels.
FETCh:MCPower:CHANnel:POWer?	Returns the reference power.
FETCh:MCPower:MAIN:CHANnels?	Returns the power of main channels.
FETCh:MCPower:SPECTrum?	Returns spectrum trace data.
FETCh:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
FETCh:MERRor:FERRor?	Returns the frequency error.
FETCh:MERRor:PEAK?	Returns the peak value.
FETCh:MERRor:PINDex?	Returns the time at the magnitude error peak.
FETCh:MERRor:RMS?	Returns the RMS value.
FETCh:MERRor:TRACe?	Returns the Magnitude error versus Time trace data.
FETCh:OBWidth subgroup	Occupied Bandwidth measurement
FETCh:OBWidth:FREQuency:ERRor?	Returns the frequency error.

Table 2-16: Fetch commands (cont.)

Header	Description
FETCh:OBWidth:OBWidth:BANDwidth?	Returns the occupied bandwidth.
FETCh:OBWidth:OBWidth:LEFT:FREQuency?	Returns the left (lower) frequency of the occupied bandwidth.
FETCh:OBWidth:OBWidth:LEFT:LEVel?	Returns the level at the left frequency of the occupied bandwidth.
FETCh:OBWidth:OBWidth:POWer?	Returns the reference power in the Occupied Bandwidth measurement.
FETCh:OBWidth:OBWidth:RIGHT:FREQuency?	Returns the right (higher) frequency of the occupied bandwidth.
FETCh:OBWidth:OBWidth:RIGHT:LEVel?	Returns the level at the right frequency of the occupied bandwidth.
FETCh:OBWidth:SPEctrum?	Returns spectrum trace data of the Occupied Bandwidth measurement.
FETCh:OBWidth:XDBBandwidth:BANDwidth?	Returns the x dB bandwidth.
FETCh:OBWidth:XDBBandwidth:LEFT:FREQuency?	Returns the left (lower) frequency of the x dB bandwidth.
FETCh:OBWidth:XDBBandwidth:LEFT:LEVel?	Returns the level at the left frequency of the x dB bandwidth.
FETCh:OBWidth:XDBBandwidth:POWer?	Returns the reference power in the x dB bandwidth measurement.
FETCh:OBWidth:XDBBandwidth:RIGHT:FREQuency?	Returns the right (higher) frequency of the x dB bandwidth.
FETCh:OBWidth:XDBBandwidth:RIGHT:LEVel?	Returns the level at the right frequency of the x dB bandwidth.
FETCh:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
FETCh:PERRor:FERRor?	Returns the frequency error.
FETCh:PERRor:PEAK?	Returns the peak value.
FETCh:PERRor:PINDex?	Returns the time at the phase error peak.
FETCh:PERRor:RMS?	Returns the RMS value.
FETCh:PERRor:TRACe?	Returns the Phase error versus Time trace data.
FETCh:PHVTime subgroup	Phase versus Time measurement
FETCh:PHVTime?	Returns the Phase versus Time trace data.
FETCh:PHVTime:MAXimum?	Returns the maximum value.
FETCh:PHVTime:MAXLocation?	Returns the time at which the phase is maximum.
FETCh:PHVTime:MINimum?	Returns the minimum value.
FETCh:PHVTime:MINLocation?	Returns the time at which the phase is minimum.
FETCh:PHVTime:RESult?	Returns the results.
FETCh:PNOise subgroup (Option 11 only)	Phase noise measurements
FETCh:PNOise:ALL?	Returns all the measurement results.
FETCh:PNOise:CARRier:FERRor?	Returns the carrier frequency error.
FETCh:PNOise:CARRier:POWer?	Returns the carrier power.
FETCh:PNOise:RESidual:FM?	Returns the residual FM.
FETCh:PNOise:RMS:PNOise?	Returns the RMS phase noise.
FETCh:PNOise:SPEctrum<x>:X?	Returns the frequencies of the specified trace.
FETCh:PNOise:SPEctrum<x>:XY?	Returns the frequency and phase noise pairs of the specified trace.
FETCh:PNOise:SPEctrum<x>:[Y]?	Returns the phase noise values of the specified trace.
FETCh:PNOise:JITTer?	Returns the jitter.
FETCh:PULSe subgroup (Option 20 only)	Pulsed RF measurements

Table 2-16: Fetch commands (cont.)

Header	Description
FETCh:PULSe[:RESult]:ATX?	Returns the average transmitted power in the results table.
FETCh:PULSe[:RESult]:AVERage?	Returns the average on power in the results table.
FETCh:PULSe[:RESult]:DRODb?	Returns the droop in dB in the pulse table.
FETCh:PULSe[:RESult]:DROop?	Returns the droop in the pulse table
FETCh:PULSe[:RESult]:DUTPct?	Returns the duty factor (%) in the results table.
FETCh:PULSe[:RESult]:DUTRatio?	Returns the duty factor (ratio) in the results table.
FETCh:PULSe[:RESult]:FALL?	Returns the fall time in the results table.
FETCh:PULSe[:RESult]:FRDeviation?	Returns the frequency deviation in the results table.
FETCh:PULSe[:RESult]:IRAmplitude?	Returns the pulse impulse response amplitude measurement in the pulse table.
FETCh:PULSe[:RESult]:IRTime?	Returns the impulse response time in the pulse table.
FETCh:PULSe[:RESult]:MFRerror?	Returns the maximum frequency error in the results table.
FETCh:PULSe[:RESult]:MPHerror?	Returns the maximum phase error in the results table.
FETCh:PULSe[:RESult]:OVEDb?	Returns the overshoot in dB in the pulse table.
FETCh:PULSe[:RESult]:OVERshoot?	Returns the overshoot in the pulse table.
FETCh:PULSe[:RESult]:PHDeviation?	Returns the phase deviation in the results table.
FETCh:PULSe[:RESult]:PPFRequency?	Returns the pulse-pulse carrier frequency in the results table.
FETCh:PULSe[:RESult]:PPOWer?	Returns the peak power in the results table.
FETCh:PULSe[:RESult]:PPPHasE?	Returns the pulse-pulse carrier phase in the results table.
FETCh:PULSe[:RESult]:RINterval?	Returns the repetition interval in the results table.
FETCh:PULSe[:RESult]:RIPDb?	Returns the ripple in dB in the pulse table.
FETCh:PULSe[:RESult]:RIPPlE?	Returns the ripple in the pulse table.
FETCh:PULSe[:RESult]:RISE?	Returns the rise time in the results table.
FETCh:PULSe[:RESult]:RMSFreqerror?	Returns the RMS frequency error in the results table.
FETCh:PULSe[:RESult]:RMSPherror?	Returns the RMS phase error in the results table.
FETCh:PULSe[:RESult]:RRATe?	Returns the repetition rate in the results table.
FETCh:PULSe[:RESult]:TIME?	Returns the time in the results table.
FETCh:PULSe[:RESult]:WIDTh?	Returns the pulse width in the results table.
FETCh:PULSe:STATistics:ATX?	Returns the average transmitted power of the statistics.
FETCh:PULSe:STATistics:AVERage?	Returns the average on power of the statistics.
FETCh:PULSe:STATistics:DRODb?	Returns the droop in dB of the statistics.
FETCh:PULSe:STATistics:DROop?	Returns the droop of the statistics
FETCh:PULSe:STATistics:DUTPct?	Returns the duty factor (%) of the statistics.
FETCh:PULSe:STATistics:DUTRatio?	Returns the duty factor (ratio) of the statistics.
FETCh:PULSe:STATistics:FALL?	Returns the fall time of the statistics.
FETCh:PULSe:STATistics:FRDeviation?	Returns the frequency deviation of the statistics.

Table 2-16: Fetch commands (cont.)

Header	Description
FETCh:PULSe:STATistics:IRAMplitude?	Returns the Pulse Impulse Response amplitude measurement in the pulse statistics.
FETCh:PULSe:STATistics:IRTime?	Returns the impulse response time in the pulse statistics.
FETCh:PULSe:STATistics:MFRqerror?	Returns the maximum frequency error of the statistics.
FETCh:PULSe:STATistics:MPHerror?	Returns the maximum phase error of the statistics.
FETCh:PULSe:STATistics:OVEdB?	Returns the overshoot measurement result in dB in the pulse statistics.
FETCh:PULSe:STATistics:OVERshoot?	Returns the overshoot measurement result in the pulse statistics.
FETCh:PULSe:STATistics:PHDeviation?	Returns the phase deviation of the statistics.
FETCh:PULSe:STATistics:PPFRrequency?	Returns the pulse-pulse carrier frequency of the statistics.
FETCh:PULSe:STATistics:PPOWER?	Returns the peak power of the statistics.
FETCh:PULSe:STATistics:PPPHase?	Returns the pulse-pulse carrier phase of the statistics.
FETCh:PULSe:STATistics:RINterval?	Returns the repetition interval of the statistics.
FETCh:PULSe:STATistics:RIPDb?	Returns the ripple in dB of the statistics.
FETCh:PULSe:STATistics:RIPple?	Returns the ripple of the statistics.
FETCh:PULSe:STATistics:RISE?	Returns the rise time of the statistics.
FETCh:PULSe:STATistics:RMSFRqerror?	Returns the RMS frequency error of the statistics.
FETCh:PULSe:STATistics:RMSPherror?	Returns the RMS phase error of the statistics.
FETCh:PULSe:STATistics:RRATe?	Returns the repetition rate of the statistics.
FETCh:PULSe:STATistics:WIDTh?	Returns the pulse width in the pulse statistics.
FETCh:PULSe:STATistics:X?	Returns the horizontal values of the trace data.
FETCh:PULSe:STATistics:XY?	Returns the horizontal and vertical values of the trace data.
FETCh:PULSe:STATistics[:Y]?	Returns the vertical values of the trace data.
FETCh:PULSe:TRACe:X?	Returns the time values of the pulse trace.
FETCh:PULSe:TRACe:XY?	Returns the horizontal (time) and vertical value pairs of the pulse trace.
FETCh:PULSe:TRACe[:Y]?	Returns the vertical values of the pulse trace.
FETCh:RFIN subgroup	All measurements
FETCh:RFIN:IQ?	Returns time-domain IQ data for a specific acquisition data record.
FETCh:RFIN:IQ:HEADer?	Returns the header information for a specific acquisition data record.
FETCh:RFIN:IQ:SCALe?	Returns the internal RF linear data scaling factor contained in the .tiq file header
FETCh:RFIN:RECOrd:IDS?	Returns the beginning and end ID numbers of acquisition data.
FETCh:SGRam subgroup	Spectrogram measurement
FETCh:SGRam?	Returns the spectrogram trace data.
FETCh:SPECTrum subgroup	Spectrum measurement
FETCh:SPECTrum:TRACe<x>?	Returns the trace data in the Spectrum Analyzer measurement.
FETCh:SPURious subgroup	Spurious measurement
FETCh:SPURious:CARRier:POWER?	Returns the carrier power.

Table 2-16: Fetch commands (cont.)

Header	Description
FETCh:SPURious:COUNT?	Returns the number of spurious signals.
FETCh:SPURious:PASS?	Returns the pass/fail limit test result.
FETCh:SPURious:SPECtrum:X?	Returns the frequencies of the spectrum trace.
FETCh:SPURious:SPECtrum:XY?	Returns the frequency and amplitude pairs of the spectrum trace.
FETCh:SPURious:SPECtrum[:Y]?	Returns the amplitudes of the spectrum trace.
FETCh:SPURious:SPUR<x>:AMPLitude:ABSolute?	Returns the absolute amplitude of the specified spurious signal.
FETCh:SPURious:SPUR<x>:AMPLitude:RELative?	Returns the relative amplitude of the specified spurious signal.
FETCh:SPURious:SPUR<x>:FREQuency:ABSolute?	Returns the absolute frequency of the specified spurious signal.
FETCh:SPURious:SPUR<x>:FREQuency:RELative?	Returns the relative frequency of the specified spurious signal.
FETCh:SPURious:SPUR<x>:LIMit:ABSolute?	Returns the absolute amplitude of the limit for a spurious signal.
FETCh:SPURious:SPUR<x>:LIMit:RELative?	Returns the relative amplitude of the limit for a spurious signal.
FETCh:SPURious:SPUR<x>:LIMit:VIOLation?	Returns whether the specified spurious signal exceeds the limit or not.
FETCh:SPURious:SPUR<x>:RANGe?	Returns the frequency range in which the spurious signal occurred.
FETCh:SQUality subgroup (Option 21 only)	Signal quality measurement
FETCh:SQUality:FREQuency:DEViation?	Returns the frequency deviation.
FETCh:SQUality:FREQuency:DEViation:TABLE?	Returns the frequency deviation measurement results table.
FETCh:SQUality:FREQuency:ERRor?	Returns the frequency error.
FETCh:SQUality:GAIN:IMBalance?	Returns the gain imbalance.
FETCh:SQUality:ORIGin:OFFSet?	Returns the origin offset.
FETCh:SQUality:PEAK:EVM?	Returns the peak EVM (%).
FETCh:SQUality:PEAK:EVM:DB?	Returns the peak EVM (dB).
FETCh:SQUality:PEAK:EVM:DB:OFFSet?	Returns the peak offset EVM (dB).
FETCh:SQUality:PEAK:EVM:LOCation?	Returns the time at which the EVM is peak.
FETCh:SQUality:PEAK:EVM:LOCation:OFFSet?	Returns the time at which the offset EVM is peak.
FETCh:SQUality:PEAK:EVM:OFFSet?	Returns the peak offset EVM (%) in the signal quality measurement.
FETCh:SQUality:PEAK:FERRor?	Returns the peak FSK error.
FETCh:SQUality:PEAK:MERRor?	Returns the peak magnitude error (%).
FETCh:SQUality:PEAK:MERRor:DB?	Returns the peak magnitude error (dB).
FETCh:SQUality:PEAK:MERRor:LOCation?	Returns the time at which the magnitude error is peak.
FETCh:SQUality:PEAK:PERRor?	Returns the peak phase error.
FETCh:SQUality:PEAK:PERRor:LOCation?	Returns the time at which the phase error is peak.
FETCh:SQUality:QUADrature:ERRor?	Returns the quadrature error.
FETCh:SQUality:RHO?	Returns the r (waveform quality).
FETCh:SQUality:RMS:EVM?	Returns the RMS EVM (%).
FETCh:SQUality:RMS:EVM:DB?	Returns the RMS EVM (dB).
FETCh:SQUality:RMS:EVM:DB:OFFSet?	Returns the RMS offset EVM (dB).
FETCh:SQUality:RMS:EVM:OFFSet?	Returns the RMS offset EVM (%).

Table 2-16: Fetch commands (cont.)

Header	Description
FETCh:SQUality:RMS:FERRor?	Returns the RMS FSK error.
FETCh:SQUality:RMS:MER:DB?	Returns the RMS MER (dB).
FETCh:SQUality:RMS:MERRor?	Returns the RMS magnitude error (%).
FETCh:SQUality:RMS:MERRor:DB?	Returns the RMS magnitude error (dB).
FETCh:SQUality:RMS:PERRor?	Returns the RMS phase error.
FETCh:SQUality:SYMBol:LENGth?	Returns the number of analyzed symbols.
FETCh:SQUality:SYMBol:RATE?	Returns the value of the calculated symbol rate.
FETCh:SQUality:SYMBol:RATE:ERRor?	Returns the value of the symbol rate error.
FETCh:TDIagram subgroup (Option 21 only)	Trellis diagram
FETCh:TDIagram:FERRor?	Returns the frequency error.
FETCh:TDIagram:TRACe?	Returns the Trellis diagram trace data.
FETCh:TOVerview subgroup	Time overview
FETCh:TOVerview?	Returns the trace data.

Initiate Commands

Use the INITiate commands to control the acquisition of data.

Table 2-17: Initiate commands

Header	Description
INITiate:CONTinuous	Sets or queries whether to acquire data continuously.
INITiate[:IMMediate]	Starts data acquisition.

Input Commands

Use the INPut commands to control the characteristics of the signal input.

Table 2-18: Input commands

Header	Description
<code>INPut:CORRection:EXTErnal:EDIT<x>:INTerpolation</code>	Sets or queries the interpolation setting to use with the indicated external gain table.
<code>INPut:CORRection:EXTErnal:EDIT<x>:NEW</code>	Creates the indicated (x) external loss table.
<code>INPut:CORRection:EXTErnal:TYPE</code>	Sets or queries the data type to use when applying the external loss table corrections.
<code>INPut:{MLEVel RLEVel}</code>	Sets or queries the reference level.
<code>INPut[:RF]:ATTenuation</code>	Sets or queries the input attenuation.
<code>INPut[:RF]:ATTenuation:AUTO</code>	Sets or queries whether to set the attenuation automatically.
<code>INPut[:RF]:ATTenuation:MONitor:STATE</code>	Sets or queries whether to enable to monitor attenuator use.
<code>INPut[:RF]:GAIN:STATE</code> (Option 01 only)	Sets or queries whether to enable the internal preamplifier.

Mass Memory Commands

Use the MMEMory commands to manipulate files on the mass memory devices.

For the trace specifier TRACe<x>, refer to *Trace Mnemonics*. (See page 2-75.)

Table 2-19: Mass memory (MMEMory) commands

Header	Description
MMEMory:{AM FM PM} subgroup	AM/FM/PM measurement
MMEMory:{AM FM PM}:LOAD:TRACe	Loads trace data from the specified file.
MMEMory:{AM FM PM}:SHOW:TRACe<x>	Enables display of a recalled trace file.
MMEMory:{AM FM PM}:STORE:TRACe	Stores trace data in the specified file.
MMEMory:AVTime subgroup	Amplitude versus Time measurement
MMEMory:AVTime:LOAD:TRACe<x>	Loads trace data from the specified file.
MMEMory:AVTime:SHOW:TRACe<x>	Enables display of a recalled trace file.
MMEMory:AVTime:STORE:TRACe<x>	Stores trace data in the specified file.
MMEMory:CALibration subgroup	Measurement calibration
MMEMory:CALibration:LOAD:CORRection:EXTErnal:EDIT<x>	Loads the external loss table data from a specified file.
MMEMory:CALibration:STORE:CORRection:EXTErnal:EDIT<x>	Stores an external loss table to a specified file.
MMEMory:CCDF subgroup	CCDF measurement
MMEMory:CCDF:LOAD:TRACe<x>	Loads trace data from the specified file.
MMEMory:CCDF:SHOW:TRACe<x>	Enables display of a recalled trace file.
MMEMory:CCDF:STORE:TRACe<x>	Stores trace data in the specified file.
MMEMory:DDEMod subgroup	DPX spectrum measurement
MMEMory:DDEMod:LOAD:FILTER:MEASurement:USER<x>	Loads a user-defined measurement filter from the specified file.
MMEMory:DDEMod:LOAD:FILTER:MEASurement:UOTHer	Loads a user-defined measurement filter from the specified file.
MMEMory:DDEMod:LOAD:FILTER:REFerence:USER<x>	Loads the specified user-defined reference filter.
MMEMory:DDEMod:LOAD:FILTER:REFerence:UOTHer	Loads the specified user-defined reference filter
MMEMory:DDEMod:LOAD:SYMBOL:MAP	Loads the specified symbol map filename.
MMEMory:DPSA subgroup	DPX spectrum measurement
MMEMory:DPSA:LOAD:TRACe<x>	Loads trace data from the specified file.
MMEMory:DPSA:SHOW:TRACe<x>	Enables display of a recalled trace file.
MMEMory:DPSA:STORE:TRACe<x>	Stores trace data in the specified file.
MMEMory:FVTime subgroup	Frequency versus Time measurement
MMEMory:FVTime:LOAD:TRACe	Loads trace data from the specified file.
MMEMory:FVTIME:SHOW:TRACe<x>	Enables display of a recalled trace file.

Table 2-19: Mass memory (MMEMory) commands (cont.)

Header	Description
MMEMory:FVTime:STORe:TRACe	Stores trace data in the specified file.
MMEMory:IQVTime subgroup	RF I&Q versus Time measurement
MMEMory:IQVTime:LOAD:TRACe:I	Loads I trace data from the specified file.
MMEMory:IQVTime:LOAD:TRACe:Q	Loads Q trace data from the specified file.
MMEMory:IQVTIME:SHOW:TRACe:I	Loads trace data from the specified file.
MMEMory:IQVTIME:SHOW:TRACe<x>:Q	Enables display of a recalled trace file.
MMEMory:IQVTime:STORe:TRACe:I	Stores I trace data in the specified file.
MMEMory:IQVTime:STORe:TRACe:Q	Stores Q trace data in the specified file.
MMEMory:LOAD subgroup	Load commands
MMEMory:LOAD:IQ	Loads time-domain IQ waveform from a specified file.
MMEMory:LOAD:STAtE	Loads the instrument setup from a specified file.
MMEMory:LOAD:TRACe	Loads the trace data from a specified file.
MMEMory:PHVTime subgroup	Phase versus Time measurement
MMEMory:PHVTime:LOAD:TRACe	Loads trace data from the specified file.
MMEMory:PHVTime:SHOW:TRACe	Enables display of a recalled trace file.
MMEMory:PHVTime:STORe:TRACe	Stores trace data in the specified file.
MMEMory:PNOise subgroup	Phase noise measurement
MMEMory:PNOise:LOAD:TRACe<x>	Loads the Phase Noise trace data from the specified file.
MMEMory:PNOise:SHOW:TRACe<x>	Enables display of a recalled Phase Noise trace file.
MMEMory:PNOise:STORe:TRACe<x>	Stores the Phase Noise trace data in the specified file.
MMEMory:SGRam subgroup	Spurious measurement
MMEMory:SGRam:LOAD:TRACe	Loads the trace data from a specified file.
MMEMory:SGRam:SHOW:TRACe	Enables display of a recalled trace file.
MMEMory:SGRam:STORe:TRACe	Stores the Spectrogram trace data in the specified file.
MMEMory:SPECTrum subgroup	Spectrum measurement
MMEMory:SPECTrum:LOAD:TRACe	Loads the trace data from a specified file.
MMEMory:SPECTrum:SHOW:TRACe<x>	Enables display of a recalled trace file.
MMEMory:SPECTrum:STORe:TRACe<x>	Stores the spectrum trace data in the specified file.
MMEMory:SPURious subgroup	Spurious measurement
MMEMory:SPURious:LOAD:TABLE	Loads the spurious table from the specified file.
MMEMory:SPURious:STORe:TABLE	Stores the spurious table in the specified file.
MMEMory:STORe subgroup	Store commands
MMEMory:STORe:IQ	Saves time-domain IQ waveform in the acquisition memory to a specified file.
MMEMory:STORe:IQ:CSV	Saves time-domain IQ waveform in the acquisition memory to a specified file in the CSV (Comma Separated Values) format.

Table 2-19: Mass memory (MMEMory) commands (cont.)

Header	Description
MMEMory:STORe:IQ:MAT	Saves time-domain IQ waveform in the acquisition memory to a specified file in the MATLAB format.
MMEMory:STORe:IQ:SELEct:FRAMES	Sets or queries which frames to save when saving TIQ acquisition data files.
MMEMory:STORe:IQ:SELEct:LENGth	Sets or queries what portion of each record is saved when saving acquisition data.
MMEMory:STORe:MStAtE	Stores the measurement parameters in a specified file.
MMEMory:STORe:RESults	Stores the measurement results including measurement parameters and trace data to a specified file.
MMEMory:STORe:SCReen	Stores the measurement results in a specified file.
MMEMory:STORe:STATe	Stores the instrument setup in a specified file.
MMEMory:STORe:TRACe	Stores trace data in a specified file.
MMEMory:TOVerview subgroup	Spurious measurement
MMEMory:TOVerview:LOAD:TRACe1	Loads the trace data from a specified file.
MMEMory:TOVerview:SHOW:TRACe1	Enables display of a recalled trace file.
MMEMory:TOVerview:STORe:TRACe1	Stores the selected trace data into the specified file.

Specifying the File

For loading and storing a file, specify the file following these rules

- You can omit the file extension to load and store data. The measurement-specific extension is automatically added.
- You can use the absolute path to specify the file name. For example, specify the *SAMPLE1* file in the *My Documents* folder on the C drive as "C:\My Documents\SAMPLE1".
- If you omit the directory path, the default path is used, which is *C:\Program Files\Tektronix\RSA6100A* initially.

Once a file is saved to a different directory, the new directory will be used as the default for all load and store operations.

Output Commands

Use the OUTPut commands to control the characteristics of the signal output.

Table 2-20: Output commands

Header		Description
OUTPut:IF:{BANDwidth BWIDth}	(Option 05 only)	Sets or queries the IF output filter.
OUTPut:IF[:STATe]	(Option 05 only)	Sets or queries whether to turn on or off IF output.
OUTPut:IQ[:STATe]	(Option 05 only)	Sets or queries whether to turn on or off IQ output.
OUTPut:NOISe[:STATe]		Sets or queries whether to turn on or off 28 V DC power.

Read Commands

The READ commands acquire an input signal once in the single mode and obtain the measurement results from that data.

To fetch the measurement results from the data currently residing in the memory without acquiring the input signal, use the FETCh commands.

Table 2-21: Read commands

Header	Description
READ:ACPower subgroup	Channel power and ACPR measurement
READ:ACPower?	Returns the ACPR measurement results.
READ:ACPower:CHANnel:POWer?	Returns the average power of the main channel.
READ:ACPower:SPEctrum?	Returns spectrum trace data of the ACPR measurement.
READ:{AM FM PM} subgroup (Option 21 only)	AM/FM/PM measurement
READ:{AM FM PM}?	Returns the trace data.
READ:AM:AMINdex?	Returns the modulation index .
READ:AM:AMNegative?	Returns the negative peak modulation factor (-AM).
READ:AM:AMPositive?	Returns the positive peak modulation factor (+AM).
READ:AM:RESult?	Returns the AM measurement results.
FETCh:AM:AMINdex?	Returns the RMS modulation factor.
READ:FM:PHALf?	Returns the half peak-peak frequency deviation (Pk-Pk/2).
READ:{FM PM}:FERRor?	Returns the frequency error in the Frequency modulation and Phase modulation measurements.
READ:FM:PNEGative?	Returns the negative peak frequency deviation (-Pk).
READ:FM:PPOSitive?	Returns the positive peak frequency deviation (+Pk).
READ:FM:PTPeak?	Returns the peak-peak frequency deviation (Pk-Pk).
READ:FM:RESult?	Returns the FM measurement results.
READ:FM:RMS?	Returns the RMS frequency deviation.
READ:PM:PNEGative?	Returns the negative peak phase deviation (-Pk).
READ:PM:PPOSitive?	Returns the positive peak phase deviation (+Pk).
READ:PM:PTPeak?	Returns the peak-peak phase deviation (Pk-Pk).
READ:PM:RESult?	Returns the PM measurement results.
READ:PM:RMS?	Returns the RMS phase deviation.
READ:AVTime subgroup	Amplitude versus Time measurement
READ:AVTime:AVERage?	Returns the RMS value.
READ:AVTime:{FIRSt SECond THIRd FOURth}?	Returns the trace data.
READ:AVTime:MAXimum?	Returns the maximum value.
READ:AVTime:MAXLocation?	Returns the time at the maximum.
READ:AVTime:MINimum?	Returns the minimum value.

Table 2-21: Read commands (cont.)

Header	Description
READ:AVTime:MINLocation?	Returns the time at the minimum.
READ:AVTime:RESult?	Returns the measurement results.
READ:CCDF subgroup	CCDF measurement
READ:CCDF?	Returns the CCDF measurement results.
READ:CCDF:{FIRSt SECond THIRd}:X?	Returns the horizontal values of the specified trace.
READ:CCDF:{FIRSt SECond THIRd}:XY?	Returns the horizontal and vertical value pairs of the specified trace.
READ:CCDF:{FIRSt SECond THIRd}:Y?	Returns the vertical values of the specified trace.
READ:CONSte subgroup (Option 21 only)	Constellation measurement
READ:CONSte:FERRor?	LAST Returns the frequency error.
READ:CONSte:RESults?	Returns the constellation measurement results.
READ:CONSte:TRACe?	Returns the constellation trace data.
READ:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
READ:DDEMod:STABle?	Returns the symbol table data.
READ:DIQVtime subgroup (Option 21 only)	Demodulated I&Q versus Time measurement
READ:DIQVtime:FERRor?	Returns the frequency error.
READ:DIQVtime:I?	Returns the I versus Time trace data.
READ:DIQVtime:Q?	Returns the Q versus Time trace data.
READ:DPSA subgroup	DPX spectrum measurement
READ:DPSA:RESults:TRACe<x>?	Returns waveform data of specified trace.
READ:DPSA:TRACe:AVERAge?	Returns waveform data of the average trace.
READ:DPSA:TRACe:BITMap?	Returns trace waveform data of the bitmap trace.
READ:DPSA:TRACe:MATH?	Returns waveform data of the math trace.
READ:DPSA:TRACe:MAXimum?	Returns waveform data of the maximum trace.
READ:DPSA:TRACe:MINimum?	Returns waveform data of the minimum trace.
READ:EDlagram subgroup (Option 21 only)	Eye diagram
READ:EDlagram:FDEVIation?	Returns the frequency deviation versus Time trace data.
READ:EDlagram:FERRor?	Returns the frequency error.
READ:EDlagram:I?	Returns the I versus Time trace data.
READ:EDlagram:Q?	Returns the Q versus Time trace data.
READ:EVM subgroup (Option 21 only)	EVM versus Time measurement
READ:EVM:FERRor?	Returns the frequency error.
READ:EVM:PEAK?	Returns the peak value.
READ:EVM:PINDex?	Returns the time at the EVM peak.
READ:EVM:RMS?	Returns the RMS value.
READ:EVM:TRACe?	Returns the EVM versus Time trace data.
READ:FDVTime subgroup (Option 21 only)	Frequency deviation versus Time measurement
READ:FDVTime:FERRor?	Returns the frequency error.

Table 2-21: Read commands (cont.)

Header	Description
READ:FDVTime:TRACe?	Returns the Frequency deviation versus Time trace data.
READ:FVTime subgroup	Frequency versus Time measurement
READ:FVTime?	Returns the Frequency versus Time trace data.
READ:FVTime:MAXimum?	Returns the maximum value.
READ:FVTime:MAXLocation?	Returns the time at which the frequency drift is maximum.
READ:FVTime:MINimum?	Returns the minimum value.
READ:FVTime:MINLocation?	Returns the time at which the frequency drift is minimum.
READ:FVTime:RESult?	Returns the measurement results.
READ:IQVTime subgroup	RF I&Q versus Time measurement
READ:IQVTime:I?	Returns the I versus Time trace data.
READ:IQVTime:MAXimum?	Returns the maximum value.
READ:IQVTime:MAXLocation?	Returns the time at which the I or Q level is maximum.
READ:IQVTime:MINimum?	Returns the minimum value.
READ:IQVTime:MINLocation?	Returns the time at which the I or Q level is minimum.
READ:IQVTime:Q?	Returns the Q versus Time trace data.
READ:IQVTime:RESult?	Returns the measurement results.
READ:MCPower subgroup	MCPR measurement
READ:MCPower:ADJacent:CHANnels?	Returns the power of adjacent channels.
READ:MCPower:CHANnel:POWer?	Returns the reference power.
READ:MCPower:MAIN:CHANnels?	Returns the power of main channels.
READ:MCPower:SPECTrum?	Returns spectrum trace data.
READ:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
READ:MERRor:FERRor?	Returns the frequency error.
READ:MERRor:PEAK?	Returns the peak value.
READ:MERRor:PINDEX?	Returns the time at the magnitude error peak.
READ:MERRor:RMS?	Returns the RMS value.
READ:MERRor:TRACe?	Returns the Magnitude error versus Time trace data.
READ:OBWidth subgroup	Occupied Bandwidth measurement
READ:OBWidth:FREQuency:ERRor?	Returns the frequency error.
READ:OBWidth:OBWidth:BANDwidth?	Returns the occupied bandwidth.
READ:OBWidth:OBWidth:LEFT:FREQuency?	Returns the left (lower) frequency of the occupied bandwidth.
READ:OBWidth:OBWidth:LEFT:LEVel?	Returns the level at the left frequency of the occupied bandwidth.
READ:OBWidth:OBWidth:POWer?	Returns the reference power in the Occupied Bandwidth measurement.
READ:OBWidth:OBWidth:RIGHT:FREQuency?	Returns the right (higher) frequency of the occupied bandwidth.
READ:OBWidth:OBWidth:RIGHT:LEVel?	Returns the level at the right frequency of the occupied bandwidth.
READ:OBWidth:SPECTrum?	Returns spectrum trace data of the Occupied Bandwidth measurement.
READ:OBWidth:XDBBandwidth:BANDwidth?	Returns the x dB bandwidth.

Table 2-21: Read commands (cont.)

Header	Description
READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY?	Returns the left (lower) frequency of the x dB bandwidth.
READ:OBWidth:XDBBandwidth:LEFT:LEVEL?	Returns the level at the left frequency of the x dB bandwidth.
READ:OBWidth:XDBBandwidth:POWER?	Returns the reference power in the x dB bandwidth measurement.
READ:OBWidth:XDBBandwidth:RIGHT:FREQUENCY?	Returns the right (higher) frequency of the x dB bandwidth.
READ:OBWidth:XDBBandwidth:RIGHT:LEVEL?	Returns the level at the right frequency of the x dB bandwidth.
READ:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
READ:PERRor:FERRor?	Returns the frequency error.
READ:PERRor:PEAK?	Returns the peak value.
READ:PERRor:PINDEX?	Returns the time at the phase error peak.
READ:PERRor:RMS	Returns the RMS value.
READ:PERRor:TRACE?	Returns the Phase error versus Time trace data.
READ:PHVTime subgroup	Phase versus Time measurement
READ:PHVTime?	Returns the Phase versus Time trace data.
READ:PHVTime:MAXimum?	Returns the maximum value.
READ:PHVTime:MAXLocation?	Returns the time at which the phase is maximum.
READ:PHVTime:MINimum?	Returns the minimum value.
READ:PHVTime:MINLocation?	Returns the time at which the phase is minimum.
READ:PHVTime:RESult?	Returns the results.
READ:PNOise subgroup (Option 11 only)	Phase noise measurements
READ:PNOise:ALL?	Returns all the measurement results.
READ:PNOise:CARRIER:FERRor?	Returns the carrier frequency error.
READ:PNOise:CARRIER:POWER?	Returns the carrier power.
READ:PNOise:RESidual:FM?	Returns the residual FM.
READ:PNOise:RMS:PNOise?	Returns the RMS phase noise.
READ:PNOise:SPECTrum<x>:X?	Returns the frequencies of the specified trace.
READ:PNOise:SPECTrum<x>:XY?	Returns the frequency and phase noise pairs of the specified trace.
READ:PNOise:SPECTrum<x>[:Y]?	Returns the phase noise values of the specified trace.
READ:PNOise:JITTER?	Returns the jitter.
READ:PULSE subgroup (Option 20 only)	Pulsed RF measurements
READ:PULSE[:RESult]:ATX?	Returns the average transmitted power in the results table.
READ:PULSE[:RESult]:AVERAGE?	Returns the average on power in the results table.
READ:PULSE[:RESult]:DRODb?	Returns the droop in dB in the pulse table.
READ:PULSE[:RESult]:DROOp?	Returns the droop in the pulse table.
READ:PULSE[:RESult]:DUTPct?	Returns the duty factor (%) in the results table.
READ:PULSE[:RESult]:DUTRatio?	Returns the duty factor (ratio) in the results table.
READ:PULSE[:RESult]:FALL?	Returns the fall time in the results table.
READ:PULSE[:RESult]:FRDeviation?	Returns the frequency deviation in the results table.

Table 2-21: Read commands (cont.)

Header	Description
READ:PULSef:RESultj:IRAMplitude?	Returns the pulse impulse response amplitude in the pulse table.
READ:PULSef:RESultj:IRTime?	Returns the impulse response time in the pulse table.
READ:PULSef:RESultj:MFReqerror?	Returns the maximum frequency error in the results table.
READ:PULSef:RESultj:MPHerror?	Returns the maximum phase error in the results table.
READ:PULSef:RESultj:OVEDb?	Returns the overshoot in dB in the pulse table.
READ:PULSef:RESultj:OVERshoot?	Returns the overshoot in the pulse table.
READ:PULSef:RESultj:PHDeviation?	Returns the phase deviation in the results table.
READ:PULSef:RESultj:PPFRequency?	Returns the pulse-pulse carrier frequency in the results table.
READ:PULSef:RESultj:PPOWer?	Returns the peak power in the results table.
READ:PULSef:RESultj:PPPHasE?	Returns the pulse-pulse carrier phase in the results table.
READ:PULSef:RESultj:RINTerval?	Returns the repetition interval in the results table.
READ:PULSef:RESultj:RIPDb?	Returns the ripple in dB in the pulse table.
READ:PULSef:RESultj:RIPple?	Returns the ripple in the results table.
READ:PULSef:RESultj:RISE?	Returns the rise time in the results table.
READ:PULSef:RESultj:RMSFreqerror?	Returns the RMS frequency error in the results table.
READ:PULSef:RESultj:RMSPherror?	Returns the RMS phase error in the results table.
READ:PULSef:RESultj:RRATe?	Returns the repetition rate in the results table.
READ:PULSef:RESultj:TIME?	Returns the time in the results table.
READ:PULSef:RESultj:WIDTh?	Returns the pulse width in the results table.
READ:PULSe:STATistics?	Returns the trace data of the pulse statistics measurement.
READ:PULSe:STATistics:ATX?	Returns the average transmitted power of the statistics.
READ:PULSe:STATistics:AVERAge?	Returns the average on power of the statistics.
READ:PULSe:STATistics:DRODb?	Returns the droop in dB of the statistics.
READ:PULSe:STATistics:DROop?	Returns the droop of the statistics.
READ:PULSe:STATistics:DUTPct?	Returns the duty factor (%) of the statistics.
READ:PULSe:STATistics:DUTRatio?	Returns the duty factor (ratio) of the statistics.
READ:PULSe:STATistics:FALL?	Returns the fall time of the statistics.
READ:PULSe:STATistics:FRDeviation?	Returns the frequency deviation of the statistics.
READ:PULSe:STATistics:IRAMplitude?	Returns the Pulse Impulse Response amplitude measurement in the pulse statistics.
READ:PULSe:STATistics:IRTime?	Returns the impulse response time in the pulse statistics.
READ:PULSe:STATistics:MFReqerror?	Returns the maximum frequency error of the statistics.
READ:PULSe:STATistics:MPHerror?	Returns the maximum phase error of the statistics.
READ:PULSe:STATistics:OVEDb?	Returns the overshoot measurement result in dB in the pulse statistics
READ:PULSe:STATistics:OVERshoot?	Returns the overshoot measurement result in the pulse statistics
READ:PULSe:STATistics:PHDeviation?	Returns the phase deviation of the statistics.
READ:PULSe:STATistics:PPFRequency?	Returns the pulse-pulse carrier frequency of the statistics.

Table 2-21: Read commands (cont.)

Header	Description
READ:PULSe:STATistics:PPOWer?	Returns the peak power of the statistics.
READ:PULSe:STATistics:PPPHase?	Returns the pulse-pulse carrier phase of the statistics.
READ:PULSe:STATistics:RINterval?	Returns the repetition interval of the statistics.
READ:PULSe:STATistics:RIPDb?	Returns the ripple in dB of the statistics
READ:PULSe:STATistics:RIPple?	Returns the ripple of the statistics.
READ:PULSe:STATistics:RISE?	Returns the rise time of the statistics.
READ:PULSe:STATistics:RMSFreqerror?	Returns the RMS frequency error of the statistics.
READ:PULSe:STATistics:RMSPherror?	Returns the RMS phase error of the statistics.
READ:PULSe:STATistics:RRATe?	Returns the repetition rate of the statistics.
READ:PULSe:STATistics:WIDTh?	Returns the pulse width of the statistics.
READ:PULSe:STATistics:X?	Returns the horizontal values of the trace data of the pulse statistics measurement.
READ:PULSe:STATistics:XY?	Returns the horizontal and vertical values of the trace data of the pulse statistics measurement.
READ:PULSe:STATistics[:Y]?	Returns the vertical values of the trace data of the pulse statistics measurement.
READ:PULSe:TRACe:X?	Returns the time values of the pulse trace.
READ:PULSe:TRACe:XY?	Returns the horizontal (time) and vertical value pairs of the pulse trace.
READ:PULSe:TRACe[:Y]?	Returns the vertical values of the pulse trace.
READ:SGRam subgroup	Spectrogram measurement
READ:SGRam?	Returns the spectrogram trace data.
READ:SPECTrum subgroup	Spectrum measurement
READ:SPECTrum:TRACe<x>?	Returns the trace data in the Spectrum Analyzer measurement.
READ:SPURious subgroup	Spurious measurement
READ:SPURious:CARRier:POWer?	Returns the carrier power.
READ:SPURious:COUNt?	Returns the number of spurious signals.
READ:SPURious:PASS?	Returns the pass/fail limit test result.
READ:SPURious:SPECTrum:X?	Returns the frequencies of the spectrum trace.
READ:SPURious:SPECTrum:XY?	Returns the frequency and amplitude pairs of the spectrum trace.
READ:SPURious:SPECTrum[:Y]?	Returns the amplitudes of the spectrum trace.
READ:SPURious:SPUR<x>:AMPLitude:ABSolute?	Returns the absolute amplitude of the specified spurious signal.
READ:SPURious:SPUR<x>:AMPLitude:RELative?	Returns the relative amplitude of the specified spurious signal.
READ:SPURious:SPUR<x>:FREQuency:ABSolute?	Returns the absolute frequency of the specified spurious signal.
READ:SPURious:SPUR<x>:FREQuency:RELative?	Returns the relative frequency of the specified spurious signal.
READ:SPURious:SPUR<x>:LIMit:ABSolute?	Returns the absolute amplitude of the limit for a spurious signal.
READ:SPURious:SPUR<x>:LIMit:RELative?	Returns the relative amplitude of the limit for a spurious signal.
READ:SPURious:SPUR<x>:LIMit:VIOLation?	Returns whether the specified spurious signal exceeds the limit or not.

Table 2-21: Read commands (cont.)

Header	Description
READ:SPURious:SPUR<x>:RANGe?	Returns the frequency range in which the spurious signal occurred.
READ:SQUality subgroup (Option 21 only)	Signal quality measurement
READ:SQUality:FREQUency:DEViation?	Returns the frequency deviation.
READ:SQUality:FREQUency:DEViation:TABLE?	Returns the frequency deviation measurement results table.
READ:SQUality:FREQUency:ERRor?	Returns the frequency error.
READ:SQUality:GAIN:IMBalance?	Returns the gain imbalance.
READ:SQUality:ORIGin:OFFSet?	Returns the origin offset.
READ:SQUality:PEAK:EVM?	Returns the peak EVM (%).
READ:SQUality:PEAK:EVM:DB?	Returns the peak EVM (dB).
READ:SQUality:PEAK:EVM:DB:OFFSet?	Returns the peak offset EVM (dB).
READ:SQUality:PEAK:EVM:LOCation?	Returns the time at which the EVM is peak.
READ:SQUality:PEAK:EVM:LOCation:OFFSet?	Returns the time at which the offset EVM is peak.
READ:SQUality:PEAK:EVM:OFFSet?	Returns the peak offset EVM (%).
READ:SQUality:PEAK:FERRor?	Returns the peak FSK error.
READ:SQUality:PEAK:MERRor?	Returns the peak magnitude error (%).
READ:SQUality:PEAK:MERRor:DB?	Returns the peak magnitude error (dB).
READ:SQUality:PEAK:MERRor:LOCation?	Returns the time at which the magnitude error is peak.
READ:SQUality:PEAK:PERRor?	Returns the peak phase error.
READ:SQUality:PEAK:PERRor:LOCation?	Returns the time at which the phase error is peak.
READ:SQUality:QUADrature:ERRor?	Returns the quadrature error.
READ:SQUality:RHO?	Returns the r (waveform quality).
READ:SQUality:RMS:EVM?	Returns the RMS EVM (%).
READ:SQUality:RMS:EVM:DB?	Returns the RMS EVM (dB).
READ:SQUality:RMS:EVM:DB:OFFSet?	Returns the RMS offset EVM (dB).
READ:SQUality:RMS:EVM:OFFSet?	Returns the RMS offset EVM (dB).
READ:SQUality:RMS:FERRor?	Returns the RMS FSK error.
READ:SQUality:RMS:MERRor:DB?	Returns the RMS MER (dB).
READ:SQUality:RMS:MERRor?	Returns the RMS magnitude error (%).
READ:SQUality:RMS:MERRor:DB?	Returns the RMS magnitude error (dB).
READ:SQUality:RMS:PERRor?	Returns the RMS phase error.
READ:SQUality:SYMBOL:LENGth?	Returns the number of analyzed symbols.
READ:SQUality:SYMBOL:RATE?	Returns the calculated symbol rate.
READ:SQUality:SYMBOL:RATE:ERRor?	LAST Returns the value of the symbol rate error.
READ:TDIagram subgroup (Option 21 only)	Trellis diagram
READ:TDIagram:FERRor?	Returns the frequency error.
READ:TDIagram:TRACe?	Returns the Trellis diagram trace data.

Table 2-21: Read commands (cont.)

Header	Description
READ:TOVerview subgroup	Time overview
READ:TOVerview?	Returns the trace data.

Sense Commands

Use the SENSE commands to set up detailed measurement conditions.

Table 2-22: Sense commands

Header	Description
[SENSe] basic command subgroup	General analysis parameter control
[SENSe]:ACQuisition:{BANDwidth BWIDTH}	Sets or queries the acquisition bandwidth.
[SENSe]:ACQuisition:FFRame:ACTual?	Queries the actual number of Fast Frames.
[SENSe]:ACQuisition:FFRame:LIMit	Sets or queries the limit number of Fast Frames.
[SENSe]:ACQuisition:FFRame:STATe	Determines whether to enable or disable the Fast Frame.
[SENSe]:ACQuisition:MEMory:AVAILable:SAMPles?	Returns the amount of acquisition memory available in the instrument.
[SENSe]:ACQuisition:MEMory:CAPacity[:TIME]?	Returns the acquisition memory capacity.
[SENSe]:ACQuisition:MEMory:USED[:PERCent]?	Returns the percentage of the capacity used.
[SENSe]:ACQuisition:MODE	Sets or queries the acquisition mode.
[SENSe]:ACQuisition:SAMPles	Sets or queries the acquisition samples.
[SENSe]:ACQuisition:SEConds	Sets or queries the acquisition length.
[SENSe]:ANALysis:ADVanced:DITHer	Determines whether to enable or disable dithering.
[SENSe]:ANALysis:LENGth	Sets or queries the analysis length.
[SENSe]:ANALysis:LENGth:ACTual?	Queries the actual analysis length.
[SENSe]:ANALysis:LENGth:AUTO	Sets or queries whether to set the analysis length automatically.
[SENSe]:ANALysis:REFerence	Sets or queries the analysis time reference.
[SENSe]:ANALysis:STARt	Sets or queries the analysis offset time.
[SENSe]:ANALysis:STARt:AUTO	Sets or queries whether to set the analysis offset automatically.
[SENSe]:MEASurement:FREQuency	Sets or queries the measurement frequency.
[SENSe]:MEASurement:FREQuency:CENTer:LOCK	Sets or queries locking the measurement center frequency.
[SENSe]:POWer:UNITs	Sets or queries the unit of power.
[SENSe]:REANalyze	Have all measurements reanalyze the current acquisition record.
[SENSe]:ROSCillator:SOURce	Sets or queries the reference oscillator source.
[SENSe]:SPECTrum:LENGth	Sets or queries the spectrum length.
[SENSe]:SPECTrum:LENGth:ACTual?	Queries the actual spectrum length.
[SENSe]:SPECTrum:LENGth:AUTO	Sets or queries whether to set the spectrum length automatically.
[SENSe]:SPECTrum:STARt	Sets or queries the spectrum offset time.
[SENSe]:SPECTrum:TIME:MODE	Sets or queries whether to set the spectrum time automatically.
[SENSe]:USETtings	Updates the analyzer settings.
[SENSe]:ACPower subgroup	Channel power and ACPR measurement
[SENSe]:ACPower:AVERage	Sets or queries how to average waveform.
[SENSe]:ACPower:AVERage:COUNT	Sets or queries the number of traces for averaging.
[SENSe]:ACPower:{BANDwidth BWIDTH}{:RESolution}	Sets or queries the resolution bandwidth (RBW).

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:ACPower:{BANDwidth BWIDTH}{:RESolution}:ACTual?	Queries the actual resolution bandwidth (RBW).
[SENSe]:ACPower:{BANDwidth BWIDTH}{:RESolution}:AUTO	Sets or queries whether to set the RBW automatically.
[SENSe]:ACPower:{BANDwidth BWIDTH}:VIDeo	Sets or queries the video bandwidth (VBW).
[SENSe]:ACPower:{BANDwidth BWIDTH}:VIDeo:STATe	Sets or queries whether to enable the video bandwidth (VBW).
[SENSe]:ACPower:CHANnel:{BANDwidth BWIDTH}	Sets or queries the channel bandwidth.
[SENSe]:ACPower:CHANnel:FILTer	Sets or queries the adjacent channel filter.
[SENSe]:ACPower:CHANnel:PAIRs	Sets or queries the number of adjacent channel pairs.
[SENSe]:ACPower:CHANnel:SPACing	Sets or queries the channel-to-channel spacing.
[SENSe]:ACPower:CHIPrate	Sets or queries the chip rate.
[SENSe]:ACPower:CLEar:RESults	Restarts the average trace.
[SENSe]:ACPower:FREQuency	Sets or queries the center frequency.
[SENSe]:ACPower:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:ACPower:FREQuency:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.
[SENSe]:ACPower:NFLoor:STATe	Sets or queries whether to enable the correction for noise floor.
[SENSe]:ACPower:OPTimize:SPAN	Sets or queries the optimization method.
[SENSe]:ACPower:POINTs:COUNT	Sets or queries the number of trace points.
[SENSe]:ACPower:RRCRolloff	Sets or queries the filter parameter for the Root Raised Cosine filter.
[SENSe]:{AM FM PM} subgroup (Option 21 only)	AM/FM/PM measurement
[SENSe]:{AM FM PM}:{BANDwidth BWIDTH}:MEASurement	Sets measurement bandwidth for the AM, FM, or PM demodulation to analyze.
[SENSe]:{AM FM PM}:CLEar:RESults	Clears measurement results.
[SENSe]:{AM FM PM}:{MTPoints MAXTracepoints}	Sets or queries the maximum trace points.
[SENSe]:AM:DETECT:AMPLitude	Sets or queries the carrier amplitude detection method.
[SENSe]:{FM PM}:BURSt:THReshold	Sets or queries the threshold level to detect bursts.
[SENSe]:{FM PM}:FREQuency:OFFSet	Sets or queries the carrier frequency offset in the FM/PM measurement.
[SENSe]:{FM PM}:FREQuency:OFFSet:MARKer	Sets the frequency offset from selected marker or delta marker location.
[SENSe]:{FM PM}:FREQuency:SEARch:AUTO	Sets or queries whether to detect the carrier frequency automatically.
[SENSe]:PM:PHASe:OFFSet	Sets the phase offset from the selected marker location.
[SENSe]:PM:PHASe:OFFSet:MARKer	Sets the carrier frequency offset from the selected marker.
[SENSe]:PM:PHASe:SEARch:AUTO	Sets or queries whether to detect the phase automatically or manually.
[SENSe]:AVTime subgroup	Amplitude versus Time measurement
[SENSe]:AVTime:{BANDwidth BWIDTH}	Sets or queries the time-domain bandwidth filter.
[SENSe]:AVTime:{BANDwidth BWIDTH}:ACTual?	Queries the actual resolution bandwidth (RBW).
[SENSe]:AVTime:CLEar:RESults	Restarts multi-trace functions (Average and Max/Min Hold).
[SENSe]:AVTime:MAXTracepoints	Sets or queries the maximum trace points.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:AVTime:MEtHod	Sets or queries the method to set the measurement bandwidth.
[SENSe]:AVTime:SPAN	Sets or queries the frequency span.
[SENSe]:CCDF subgroup	CCDF measurement
[SENSe]:CCDF:{BANDwidth BWIDTH}	Sets or queries the CCDF measurement bandwidth.
[SENSe]:CCDF:CLear	Clears the CCDF accumulator and restarts the measurement.
[SENSe]:CCDF:TIME:TOTal:LENGth	Sets or queries the CCDF measurement time.
[SENSe]:CCDF:TIME:TYPE	Sets or queries how to repeat the CCDF measurement.
[SENSe]:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
[SENSe]:DDEMod:ANALysis:LENGth	Sets or queries the analysis length.
[SENSe]:DDEMod:ANALysis:LENGth:ACTual?	Queries the actual analysis length.
[SENSe]:DDEMod:ANALysis:LENGth:AUTO	Sets or queries whether to set the analysis length automatically.
[SENSe]:DDEMod:{BANDwidth BWIDTH}:MODE	Sets or queries the measurement bandwidth mode.
[SENSe]:DDEMod:{BANDwidth BWIDTH}:TINterval	Sets or queries the measurement bandwidth (frequency span).
[SENSe]:DDEMod:{BANDwidth BWIDTH}:TINterval:AUTO	Sets the measurement bandwidth (frequency span) automatically.
[SENSe]:DDEMod:BURSt:DEtect	Sets or queries how to detect bursts.
[SENSe]:DDEMod:BURSt:THReshold	Sets or queries the threshold level to determine a burst.
[SENSe]:DDEMod:CARRier:OFFSet	Sets or queries the carrier frequency offset.
[SENSe]:DDEMod:CARRier:OFFSet:AUTO	Sets or queries whether to detect the carrier frequency automatically.
[SENSe]:DDEMod:FILTer:ALPHa	Sets or queries the filter factor (a/BT).
[SENSe]:DDEMod:FILTer:MEASurement	Sets or queries the measurement filter.
[SENSe]:DDEMod:FILTer:REFerence	Sets or queries the reference filter.
[SENSe]:DDEMod:FREQuency:DEViation	Sets or queries the frequency deviation to determine two states for FSK.
[SENSe]:DDEMod:FREQuency:DEViation:AUTO	Sets or queries whether to detect the frequency deviation automatically.
[SENSe]:DDEMod:MAGNitude:NORMalize	Sets or queries the method for the magnitude normalization.
[SENSe]:DDEMod:MINDEX	Sets or queries the modulation index for a CPM signal.
[SENSe]:DDEMod:MINDEX:AUTO	Sets or queries whether to detect the modulation index automatically.
[SENSe]:DDEMod:MODulation:TYPE	Sets or queries the modulation type.
[SENSe]:DDEMod:PRESet	Presets the modulation analysis to a communication standard.
[SENSe]:DDEMod:SRATe	Sets or queries the symbol rate.
[SENSe]:DDEMod:SWAP:IQ	Sets or queries whether or not to swap I and Q data.
[SENSe]:DDEMod:SYMBol:HSSHift	Sets or queries the Q data half-symbol shift for OQPSK and SOQPSK signals.
[SENSe]:DDEMod:SYMBol:MAP:SOURce?	Specifies or queries the user symbol map file.
[SENSe]:DDEMod:SYMBol:MAP[:STATE]	Sets or queries whether to use the user symbol map.
[SENSe]:DDEMod:SYMBol:PLOT:POSition	Sets or queries the symbol point location on an SOQPSK waveform.
[SENSe]:DDEMod:SYMBol:POINts	Sets or queries the number of points per symbol.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:DDEMod:SYMBOL:RATE:SEARCh	Determines whether to enable a symbol rate search.
[SENSe]:DDEMod:SYNCh:WORD	Sets or queries whether to enable the synchronization word.
[SENSe]:DDEMod:SYNCh:WORD:SYMBOL	Sets or queries the synchronization word.
[SENSe]:DDEMod:TIME:UNITs	Sets or queries the fundamental unit of time.
[SENSe]:DPSA subgroup	DPX spectrum measurement
[SENSe]:DPSA:AUDio:DEMod:GAIN	Sets or queries the gain for the audio demodulation.
[SENSe]:DPSA:AUDio:DEMod:RXBWidth	Sets or queries the receiver bandwidth for the audio demodulation.
[SENSe]:DPSA:AUDio:DEMod:RXFRrequency?	Queries the receiver frequency for the audio demodulation.
[SENSe]:DPSA:AUDio:DEMod:STATE	Sets or queries whether to enable or disable the audio demodulation.
[SENSe]:DPSA:AUDio:DEMod:TUNE	Sets or queries how to determine the tuning frequency.
[SENSe]:DPSA:AUDio:DEMod:TYPE	Sets or queries the modulation type for the audio demodulation.
[SENSe]:DPSA:{BANDwidth BWIDTH}:ACTual?	Sets or queries the resolution bandwidth (RBW).
[SENSe]:DPSA:{BANDwidth BWIDTH}:OPTimization	FIRST Sets or queries the RF & IF Optimization for the Spectrum and Spectrogram displays.
[SENSe]:DPSA:{BANDwidth BWIDTH}{:RESolution}:AUTO	Determines whether to set the resolution bandwidth (RBW) automatically or manually in the DPX spectrum measurement.
[SENSe]:DPSA:FREQUENCY:SPAN: {BANDwidth BWIDTH}{:RESolution}:RATio	Sets or queries whether to set the RBW automatically.
[SENSe]:DPSA:CLEAr:RESults	Restarts multi-trace functions (Average and Max/Min Hold).
[SENSe]:DPSA:COLor	Sets or queries the color palette of three-dimensional graphs.
[SENSe]:DPSA:COLor:MINimum	Sets or queries the minimum value of the color axis.
[SENSe]:DPSA:COLor:MAXimum	Sets or queries the maximum value of the color axis.
[SENSe]:DPSA:DDENsity:MEASurement:SHOW	Sets or queries the Show measurement value (measurement always visible for DPX Trigger).
[SENSe]:DPSA:DWELI	Sets or queries the value of the Dwell time for the DPX spectrum measurement. (Option 200 only.)
[SENSe]:DPSA:DWELI:AUTO	Sets the value of the Dwell time automatically. (Option 200 only.)
[SENSe]:DPSA:POINts:COUNT	Sets or queries the number of DPX trace points.
[SENSe]:DPSA:FREQUENCY:CENTer	Sets or queries the center frequency.
[SENSe]:DPSA:FREQUENCY:SPAN	Sets or queries the frequency span.
[SENSe]:DPSA:FREQUENCY:START	Sets or queries the measurement start frequency.
[SENSe]:DPSA:FREQUENCY:STEP	Sets or queries the frequency step size.
[SENSe]:DPSA:FREQUENCY:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.
[SENSe]:DPSA:FREQUENCY:STOP	Sets or queries the measurement stop frequency.
[SENSe]:FVTime subgroup	Frequency versus Time measurement
[SENSe]:FVTime:CLEAr:RESults	Restarts multi-trace functions (Average and Max/Min Hold).
[SENSe]:FVTime:FREQUENCY:CENTer	Sets or queries the center frequency.
[SENSe]:FVTime:FREQUENCY:SPAN	Sets or queries the frequency span.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:FVTime:FREQuency:START	Sets or queries the measurement start frequency.
[SENSe]:FVTime:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:FVTime:FREQuency:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.
[SENSe]:FVTime:FREQuency:STOP	Sets or queries the measurement stop frequency.
[SENSe]:FVTime:MAXTracepoints	Sets or queries the maximum trace points.
[SENSe]:IQVTime subgroup	RF I&Q versus Time measurement
[SENSe]:IQVTime:CLEar:RESuLts	Restarts multi-trace functions (Average and Max/Min Hold).
[SENSe]:IQVTime:FREQuency:CENTer	Sets or queries the center frequency.
[SENSe]:IQVTime:FREQuency:SPAN	Sets or queries the frequency span.
[SENSe]:IQVTime:FREQuency:START	Sets or queries the measurement start frequency.
[SENSe]:IQVTime:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:IQVTime:FREQuency:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.
[SENSe]:IQVTime:FREQuency:STOP	Sets or queries the measurement stop frequency.
[SENSe]:IQVTime:MAXTracepoints	Sets or queries the maximum trace points.
[SENSe]:MCPower subgroup	MCPR measurement
[SENSe]:MCPower:AVERage	Sets or queries how to average waveform.
[SENSe]:MCPower:AVERage:COUNT	Sets or queries the number of waveforms for average.
[SENSe]:MCPower:{BANDwidth BWIDTH}[:RESolution]	Sets or queries the resolution bandwidth (RBW).
[SENSe]:MCPower:{BANDwidth BWIDTH}[:RESolution]:ACTual?	Queries the actual resolution bandwidth (RBW).
[SENSe]:MCPower:{BANDwidth BWIDTH}[:RESolution]:AUTO	Sets or queries whether to set the RBW automatically.
[SENSe]:MCPower:{BANDwidth BWIDTH}:VIDeo	Sets or queries the video bandwidth (VBW).
[SENSe]:MCPower:{BANDwidth BWIDTH}:VIDeo:STATe	Sets or queries whether to enable the video bandwidth (VBW).
[SENSe]:MCPower:CHANnel:ADJacent:ADD	Adds a pair of upper and lower adjacent channels.
[SENSe]:MCPower:CHANnel:ADJacent:DELeTe	Deletes a selected adjacent channel.
[SENSe]:MCPower:CHANnel:FILTer	Sets or queries the measurement filter.
[SENSe]:MCPower:CHANnel:MAIN:{BANDwidth BWIDTH}	Sets or queries the frequency bandwidth of the main channels.
[SENSe]:MCPower:CHANnel:MAIN:COUNT	Sets or queries the number of main channels.
[SENSe]:MCPower:CHANnel:MAIN:INACTive	Makes a main channel inactive or queries the inactive main channels.
[SENSe]:MCPower:CHANnel:MAIN:SPACing	Sets or queries the main channel spacing.
[SENSe]:MCPower:CHIPrate	Sets or queries the chip rate.
[SENSe]:MCPower:CLEar:RESuLts	Restarts the average trace.
[SENSe]:MCPower:FREQuency	Sets or queries the center frequency.
[SENSe]:MCPower:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:MCPower:FREQuency:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:MCPower:NFLoor:STATe	Sets or queries whether to enable the correction for noise floor.
[SENSe]:MCPower:OPTimize:SPAN	Sets or queries the optimization method.
[SENSe]:MCPower:POINTs:COUNT	Sets or queries the number of trace points.
[SENSe]:MCPower:RCHannels?	Queries the power reference.
[SENSe]:MCPower:RCHannels:MAIN<x>	Sets the power reference to the main channel with the index (<x>).
[SENSe]:MCPower:RCHannels:TOTal	Sets the power reference to the total power of all the active channels.
[SENSe]:MCPower:RRCRolloff	Sets or queries the filter parameter for the Root Raised Cosine filter.
[SENSe]:OBWidth subgroup	Occupied Bandwidth measurement
[SENSe]:OBWidth:AVERage	Sets or queries whether to enable or disable averaging.
[SENSe]:OBWidth:AVERage:COUNT	Sets or queries the number of measurements for averaging.
[SENSe]:OBWidth:{BANDwidth BWIDTH}:MEASurement	Sets or queries the measurement bandwidth.
[SENSe]:OBWidth:{BANDwidth BWIDTH}[:RESolution]	Sets or queries the resolution bandwidth (RBW).
[SENSe]:OBWidth:{BANDwidth BWIDTH}[:RESolution]:ACTual?	Queries the actual resolution bandwidth (RBW).
[SENSe]:OBWidth:{BANDwidth BWIDTH}[:RESolution]:AUTO	Sets or queries whether to set the RBW automatically.
[SENSe]:OBWidth:{BANDwidth BWIDTH}:VIDeo	Sets or queries the video bandwidth (VBW).
[SENSe]:OBWidth:{BANDwidth BWIDTH}:VIDeo:STATe	Sets or queries whether to enable the video bandwidth (VBW).
[SENSe]:OBWidth:CLEar:RESults	Restarts the averaging.
[SENSe]:OBWidth:FREQuency:CENTer	Sets or queries the center frequency.
[SENSe]:OBWidth:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:OBWidth:FREQuency:STEP:AUTO	Determines whether to set the frequency step size automatically.
[SENSe]:OBWidth:PERCent	Sets or queries the occupied bandwidth percent power.
[SENSe]:OBWidth:XDBLevel	Sets or queries the x dB level.
[SENSe]:PHVTime subgroup	Phase versus Time measurement
[SENSe]:PHVTime:CLEar:RESults	Restarts multi-trace functions (Average and Max/Min Hold).
[SENSe]:PHVTime:FREQuency:CENTer	Sets or queries the center frequency.
[SENSe]:PHVTime:FREQuency:SPAN	Sets or queries the frequency span.
[SENSe]:PHVTime:FREQuency:START	Sets or queries the measurement start frequency.
[SENSe]:PHVTime:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:PHVTime:FREQuency:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.
[SENSe]:PHVTime:FREQuency:STOP	Sets or queries the measurement stop frequency.
[SENSe]:PHVTime:MAXTracepoints	Sets or queries the maximum trace points.
[SENSe]:PNOise subgroup (Option 11 only)	Phase noise measurement
[SENSe]:PNOise:AVERage:COUNT	Sets or queries the number of traces to combine for averaging.
[SENSe]:PNOise:AVERage:ENABLE	Sets or queries whether to enable or disable averaging trace.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:PNOise:CARRier:FREQuency:TRACk	Sets or queries whether to enable tracking the carrier frequency.
[SENSe]:PNOise:CARRier:THReshold	Sets or queries the threshold level to detect the carrier.
[SENSe]:PNOise:CLEar:RESults	Restarts the average process.
[SENSe]:PNOise:FREQuency:INTegration:OFFSet:START	Sets or queries the start offset frequency for integration.
[SENSe]:PNOise:FREQuency:INTegration:OFFSet:STOP	Sets or queries the stop offset frequency for integration.
[SENSe]:PNOise:FREQuency:PLOT:OFFSet:START	Sets or queries the start offset frequency for plot.
[SENSe]:PNOise:FREQuency:PLOT:OFFSet:STOP	Sets or queries the stop offset frequency for plot.
[SENSe]:PNOise:OPTimization	Sets or queries the method of optimization.
[SENSe]:PULSe subgroup (Option 20 only)	Pulsed RF measurements
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:ALENght	Sets or queries the absolute amount of time included in the Frequency-Domain Linearity measurements.
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:METHod	Sets or queries the measurement time method for the Frequency-Domain Linearity measurements.
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:RLENght	Sets or queries the relative amount of time included in the Frequency-Domain Linearity measurements.
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:RLEVel	Sets or queries the Frequency-Domain Linearity measurement reference level.
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:START	Sets or queries the start time for the Frequency-Domain Linearity measurements
[SENSe]:PULSe:ANALyze:IREsponse:CORRection:AMPLitude[:STATe]	Enables or disables the impulse response measurement amplitude corrections for window and for delay of the highest side lobe.
[SENSe]:PULSe:ANALyze:IREsponse:KOTime	Sets or queries the impulse response measurement Keep-out time.
[SENSe]:PULSe:ANALyze:IREsponse:MEASurement:TIME:ALENght	Sets or queries the absolute amount of time included in impulse response measurements.
[SENSe]:PULSe:ANALyze:IREsponse:MEASurement:TIME:METHod	Sets or queries the impulse response measurement time method.
[SENSe]:PULSe:ANALyze:IREsponse:MEASurement:TIME:RLENght	Sets or queries the relative amount of time included in Impulse Response measurements.
[SENSe]:PULSe:ANALyze:IREsponse:MEASurement:TIME:RLEVel	Sets or queries the measurement reference level for Impulse Response measurements.
[SENSe]:PULSe:ANALyze:IREsponse:MEASurement:TIME:START	Sets or queries the start time for the Impulse Response measurements.
[SENSe]:PULSe:ANALyze:LEVel	Sets or queries how to determine the 50% level.
[SENSe]:PULSe:ANALyze:LEVel:FIFTy	Sets or queries how to determine the 50% level.
[SENSe]:PULSe:ANALyze:LEVel:HUNDred	Sets or queries how to determine the 50% level.
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:ALENght	Sets or queries the absolute amount of time included in the Overshoot measurements.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:METHod	Sets or queries the measurement time method for the Overshoot measurements.
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RENgth	Sets or queries the relative amount of time included in the Overshoot measurements.
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEVel	Sets or queries the measurement reference level for the Overshoot measurements.
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:STARt	Sets or queries the start time for the Overshoot measurements
[SENSe]:PULSe:ANALyze:PMLocation	Sets or queries the phase measurement location.
[SENSe]:PULSe:ANALyze:POINt:LOCation	Sets or queries the point location method.
[SENSe]:PULSe:ANALyze:RFALl	Sets or queries the threshold levels to measure the rise/fall time.
[SENSe]:PULSe:ANALyze:RIPPlE	Sets or queries the ripple portion of the pulse top.
[SENSe]:PULSe:CARRier:FREQUency?	Queries the carrier frequency.
[SENSe]:PULSe:CARRier:OFFSet	Sets or queries the carrier frequency offset.
[SENSe]:PULSe:CARRier:SEARCh	Sets or queries how to detect the carrier.
[SENSe]:PULSe:DETEct:MEASurement	Sets or queries whether to set the maximum number of pulses.
[SENSe]:PULSe:DETEct:NUMBer	Sets or queries the maximum number of pulses to detect.
[SENSe]:PULSe:DETEct:POWer[:THREshold]	Sets or queries the power threshold to detect pulses.
[SENSe]:PULSe:DETEct:TIME[:THREshold]	Sets or queries the minimum off-time between pulses.
[SENSe]:PULSe:FILTer:{BANDwidth BWIDTH}	Sets or queries the filter bandwidth for the Gaussian filter.
[SENSe]:PULSe:FILTer:MEASurement	Sets or queries the measurement filter.
[SENSe]:PULSe:FREFerence:AUTO	Determines whether to estimate the frequency reference automatically.
[SENSe]:PULSe:FREFerence:CSLoPe	Sets or queries the Chirp Slope.
[SENSe]:PULSe:FREFerence:CSLoPe:AUTO	Sets or queries enabling automatic Chirp Slope estimating.
[SENSe]:PULSe:FREFerence:OFFSet	Sets or queries the frequency reference offset.
[SENSe]:PULSe:MODulation:TYPE	Sets or queries the modulation type.
[SENSe]:PULSe:SIGNAL:TYPE	Sets or queries the signal type in the pulsed RF measurements.
[SENSe]:PULSe:STATistics:HISTogram:ORDinate	Sets or queries the Histogram Y unit.
[SENSe]:PULSe:STATistics:HISTogram:POINts	Sets or queries the number of bins in the Histogram plot.
[SENSe]:PULSe:STATistics:HISTogram:POINts:AUTO	Sets or queries enabling automatic Histogram plot bins count.
[SENSe]:REANalyze subgroup	Spectrogram measurement
[SENSe]:REANalyze	Sets all measurements to reanalyze the current acquisition record.
[SENSe]:REANalyze:ACQuisition:SETTings?	Queries the settings of all acquisitions in acquisition history.
[SENSe]:REANalyze:ALL	Replay all items in the current acquisition history selection.
[SENSe]:REANalyze:CURRent	Replay the current item in acquisition history selection.
[SENSe]:REANalyze:CURRent:ACQuisition?	Queries the Acquisition record identifier (ID) of the current (last) reanalyzed record.
[SENSe]:REANalyze:CURRent:FRAMe?	Queries the Frame identifier (ID) of the current (last) reanalyzed record.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:REANalyze:CURRent:TIMestamp?	Queries the timestamp of the current (last) reanalyzed record.
[SENSe]:REANalyze:DELeTe:DATA	Deletes all data in the acquisition history.
[SENSe]:REANalyze:FIRSt	Replays the first item in the current acquisition history selection.
[SENSe]:REANalyze:LAST	Replays the last item in the current acquisition history selection.
[SENSe]:REANalyze:NEXt	Replays the next item in the current acquisition history selection.
[SENSe]:REANalyze:PAUSe	Sets or queries the reanalysis pause state.
[SENSe]:REANalyze:PREVious	Replays the previous item in the current Replay selection.
[SENSe]:REANalyze:SELEct:ACQuisition:FIRSt?	Queries the first selectable acquisition history Start or Stop value.
[SENSe]:REANalyze:SELEct:ACQuisition:FIRSt:TIMestamp?	Queries the timestamp associated with the first selectable acquisition history Start or Stop value.
[SENSe]:REANalyze:SELEct:ACQuisition:LAST?	Queries the last selectable acquisition history Start or Stop value.
[SENSe]:REANalyze:SELEct:ACQuisition:LAST:TIMestamp?	Queries the timestamp associated with the last selectable acquisition history Start or Stop value.
[SENSe]:REANalyze:SELEct:ACQuisition:START	Sets or queries the Acquisition Start value in the acquisition history selection.
[SENSe]:REANalyze:SELEct:ACQuisition:START:TIMestamp?	Queries the timestamp associated with the current Acquisition Start selection.
[SENSe]:REANalyze:SELEct:ACQuisition:STOP	Sets or queries the Acquisition Stop value in the acquisition history selection.
[SENSe]:REANalyze:SELEct:ACQuisition:STOP:TIMestamp?	Queries the timestamp associated with the current Acquisition Stop selection.
[SENSe]:REANalyze:SELEct:ALL	Selects all acquisitions and frames in the current acquisition history.
[SENSe]:REANalyze:SELEct:FRAMe:FIRSt?	Queries the first available Frame Start or Stop value available for acquisition history selection.
[SENSe]:REANalyze:SELEct:FRAMe:FIRSt:TIMestamp?	Queries the timestamp associated with the first available frame of the first available Acquisition Start or Stop value.
[SENSe]:REANalyze:SELEct:FRAMe:LAST?	Queries the last available Frame Start or Stop value available for acquisition history selection.
[SENSe]:REANalyze:SELEct:FRAMe:LAST:TIMestamp?	Queries the timestamp associated with the last available frame of the last available Acquisition Start or Stop value.
[SENSe]:REANalyze:SELEct:FRAMe:START	Sets or queries the Frame Start value in the acquisition history selection.
[SENSe]:REANalyze:SELEct:FRAMe:START:TIMestamp?	Queries the timestamp associated with the current Frame Start selection.
[SENSe]:REANalyze:SELEct:FRAMe:STOP	Sets or queries the frame stop value in acquisition history selection.
[SENSe]:REANalyze:SELEct:FRAMe:STOP:TIMestamp?	Queries the timestamp associated with the current frame stop selection.
[SENSe]:REANalyze:SPEEd	Sets or queries the time delay value inserted between reanalysis of frames or acquisitions.
[SENSe]:REANalyze:STOP	Stops the current reanalysis.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:REANalyze:TIMestamp:DECimal	Sets or queries the number of values to the right of the decimal point to include in all timestamps.
[SENSe]:ROSCillator subgroup	All measurements
[SENSe]:ROSCillator:SOURce	Sets or queries the frequency reference oscillator source.
[SENSe]:SGRam subgroup	Spectrogram measurement
[SENSe]:SGRam:{BANDwidth BWIDth}:OPTimization	Sets or queries the method of optimizing gain and input bandwidth.
[SENSe]:SGRam:{BANDwidth BWIDth}:RESolution	Sets or queries the resolution bandwidth (RBW).
[SENSe]:SGRam:{BANDwidth BWIDth}[:RESolution]:ACTual?	Queries the actual resolution bandwidth (RBW).
[SENSe]:SGRam:{BANDwidth BWIDth}[:RESolution]:AUTO	Sets or queries whether to set the RBW automatically.
[SENSe]:SGRam:{BANDwidth BWIDth}[:RESolution]:MODE	Sets or queries whether to enable or disable the RBW processing.
[SENSe]:SGRam:{BANDwidth BWIDth}:VIDeo	Sets or queries the video bandwidth (VBW).
[SENSe]:SGRam:{BANDwidth BWIDth}:VIDeo:STATe	Sets or queries whether to enable the video bandwidth (VBW).
[SENSe]:SGRam:COLor	Sets or queries the color palette of three-dimensional graphs.
[SENSe]:SGRam:COLor:MAXimum	Sets or queries the maximum value of the color axis.
[SENSe]:SGRam:COLor:MINimum	Sets or queries the minimum value of the color axis.
[SENSe]:SGRam:FFT:WINDow	Sets or queries the FFT window.
[SENSe]:SGRam:FILTer[:SHAPe]	Sets or queries the filter shape.
[SENSe]:SGRam:FREQuency:CENTer	Sets or queries the center frequency.
[SENSe]:SGRam:FREQuency:SPAN	Sets or queries the frequency span.
[SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:RESolution]:RATio	Sets or queries the ratio of span to RBW.
[SENSe]:SGRam:FREQuency:SPAN:MAXimum	Sets the frequency range to the maximum real-time span.
[SENSe]:SGRam:FREQuency:START	Sets or queries the measurement start frequency.
[SENSe]:SGRam:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:SGRam:FREQuency:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.
[SENSe]:SGRam:FREQuency:STOP	Sets or queries the measurement stop frequency.
[SENSe]:SPECtrum subgroup	Spectrum measurement
[SENSe]:SPECtrum:{BANDwidth BWIDth}:OPTimization	Sets or queries the method of optimizing gain and input bandwidth.
[SENSe]:SPECtrum:{BANDwidth BWIDth}[:RESolution]	Sets or queries the resolution bandwidth (RBW).
[SENSe]:SPECtrum:{BANDwidth BWIDth}[:RESolution]:ACTual?	Queries the actual resolution bandwidth (RBW).
[SENSe]:SPECtrum:{BANDwidth BWIDth}[:RESolution]:AUTO	Sets or queries whether to set the RBW automatically.

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]:MODE	Sets or queries whether to enable or disable the RBW process.
[SENSe]:SPECTrum:{BANDwidth BWIDth}:VIDeo	Sets or queries the video bandwidth (VBW).
[SENSe]:SPECTrum:{BANDwidth BWIDth}:VIDeo:STATe	Sets or queries whether to enable the video bandwidth (VBW).
[SENSe]:SPECTrum:CLEar:RESults	Restarts multi-trace functions (Average and Max/Min Hold).
[SENSe]:SPECTrum:FFT:WINDow	Sets or queries the FFT window.
[SENSe]:SPECTrum:FILTer[:SHAPE]	Sets or queries the filter shape.
[SENSe]:SPECTrum:FREQuency:CENTer	Sets or queries the center frequency.
[SENSe]:SPECTrum:FREQuency:SPAN	Sets or queries the frequency span.
[SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATIo	Sets or queries the ratio of span to RBW.
[SENSe]:SPECTrum:FREQuency:START	Sets or queries the measurement start frequency.
[SENSe]:SPECTrum:FREQuency:STEP	Sets or queries the frequency step size.
[SENSe]:SPECTrum:FREQuency:STEP:AUTO	Sets or queries whether to set the frequency step size automatically.
[SENSe]:SPECTrum:FREQuency:STOP	Sets or queries the measurement stop frequency.
[SENSe]:SPECTrum:LENGth	Sets or queries the spectrum length.
[SENSe]:SPECTrum:LENGth:ACTual?	Queries the actual spectrum length.
[SENSe]:SPECTrum:LENGth:AUTO	Sets or queries the spectrum length mode (automatic or manual).
[SENSe]:SPECTrum:MAX:SPAN	Sets the frequency span to the maximum span.
[SENSe]:SPECTrum:POINts:COUNT	Sets or queries the number of sample points on the signal spectrum.
[SENSe]:SPECTrum:START	Sets or queries the spectrum offset time
[SENSe]:SPECTrum:TIME:MODE	Sets or queries the spectrum time parameter mode (automatic or manual).
[SENSe]:SPURious subgroup	Spurious measurement
[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}	Sets or queries the channel width for the carrier as power reference.
[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}:INTegration	Sets or queries the integration bandwidth to calculate the carrier power.
[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}[:RESolution]	Sets or queries the resolution bandwidth to measure the carrier power.
[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}[:RESolution]:AUTO	Sets or queries whether to set the resolution bandwidth automatically.
[SENSe]:SPURious:CARRier:DETection	Sets or queries the carrier detection method.
[SENSe]:SPURious:CARRier:FREQuency	Sets or queries the carrier frequency.
[SENSe]:SPURious:CARRier:THReshold	Sets or queries the threshold level to detect the carrier.
[SENSe]:SPURious:CLEar:RESults	Restarts multi-trace functions (Average and Max Hold).
[SENSe]:SPURious[:FREQuency]:OVERlap?	Queries whether any of the frequency ranges (A to T) overlap.
[SENSe]:SPURious:LIST	Sets or queries how to list the spurious signals.
[SENSe]:SPURious:MODE	Sets or queries the frequency range mode (Multi or Single).

Table 2-22: Sense commands (cont.)

Header	Description
[SENSe]:SPURious:OPTimization	Sets or queries the method of optimization.
[SENSe]:SPURious:POINts:COUNT	Sets or queries the trace point count for the frequency range.
[SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo	Sets or queries the VBW for the specified frequency range.
[SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo:STATe	Sets or queries whether to enable the VBW for the frequency range.
[SENSe]:SPURious:RANGe<x>:DETection	Sets or queries the display detector for the frequency range.
[SENSe]:SPURious:RANGe<x>:EXCursion	Sets or queries the excursion level in the frequency range.
[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]	Sets or queries the filter shape for the frequency range.
[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]:BANDwidth	Sets or queries the filter bandwidth for the frequency range.
[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]:BANDwidth:AUTO	Sets or queries whether to set the filter bandwidth automatically.
[SENSe]:SPURious:RANGe<x>:FREQuency:START	Sets or queries the start frequency of the range.
[SENSe]:SPURious:RANGe<x>:FREQuency:STOP	Sets or queries the stop frequency of the range.
[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:START	Sets or queries the absolute start amplitude of the limits for the range.
[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:STOP	Sets or queries the absolute stop amplitude of the limits for the range.
[SENSe]:SPURious:RANGe<x>:LIMit:MASK	Sets or queries the limit mask function mode for the frequency range.
[SENSe]:SPURious:RANGe<x>:LIMit:RELative:START	Sets or queries the relative start amplitude of the limits for the range.
[SENSe]:SPURious:RANGe<x>:LIMit:RELative:STOP	Sets or queries the relative stop amplitude of the limits for the range.
[SENSe]:SPURious:RANGe<x>:STATe	Sets or queries whether to enable or disable the frequency range.
[SENSe]:SPURious:RANGe<x>:THReshold	Sets or queries the threshold level to detect spurious signals in a range.
[SENSe]:SPURious:REFerence	Sets or queries the power reference.
[SENSe]:SPURious:REFerence:MANual:POWer	Sets or queries the reference power level.
[SENSe]:TOVerview subgroup	Time overview
[SENSe]:TOVerview:FREQuency:CENTer	Sets or queries the center frequency.
[SENSe]:TOVerview:MAXTracepoints	Sets or queries the maximum trace points.
[SENSe]:USETtings subgroup	All measurements
[SENSe]:USETtings	Updates the analyzer settings.

Status Commands

Use the STATus commands to control registers defined in the SCPI status reporting structure.

Table 2-23: Status commands

Header	Description
STATus:ACPower:EVENTs?	Returns the current events for the ACPR measurement.
STATus:{AM FM PM}:EVENTs?	Returns the current events for the AM/FM/PM measurement.
STATus:AVTime:EVENTs?	Returns the current events for the Amplitude versus Time measurement.
STATus:CCDF:EVENTs?	Returns the current events for the CCDF measurement.
STATus:CONStellation:EVENTs?	Returns the current events for the Constellation measurement.
STATus:DIQTime:EVENTs?	Returns the current events for the Demod I&Q versus Time measurement.
STATus:DPXSA:EVENTs?	Returns the current events for the DPX spectrum measurement.
STATus:EDIagram:EVENTs?	Returns the current events for the Eye diagram measurement.
STATus:EVM:EVENTs?	Returns the current events for the EVM versus Time measurement.
STATus:FDVTime:EVENTs?	Returns the current events for the Freq dev versus Time measurement.
STATus:FVTime:EVENTs?	Returns the current events for the Frequency versus Time measurement.
STATus:IQVTime:EVENTs?	Returns the current events for the RF I&Q versus Time measurement.
STATus:MCPR:EVENTs?	Returns the current events for the MCPR measurement.
STATus:MERRor:EVENTs?	Returns the current events for the Mag error versus Time measurement.
STATus:OBWidth:EVENTs?	Returns the current events for the Occupied Bandwidth measurement.
STATus:OPERation:CONDition?	Queries the contents of the OCR.
STATus:OPERation:ENABle	Sets or queries the mask for the OENR.
STATus:OPERation[:EVENT]?	Queries the contents of the OEVR.
STATus:OPERation:NTRansition	Sets or queries the value of the negative transition filter.
STATus:OPERation:PTRansition	Sets or queries the value of the positive transition filter.
STATus:PERRor:EVENTs?	Returns the current events for the Phase error measurement.
STATus:PHVTime:EVENTs?	Returns the current events for the Phase versus Time measurement.
STATus:PNOise:EVENTs?	Returns the current events for the phase noise measurement.
STATus:PRESet	Presets a status byte.
STATus:PULSe:RESult:EVENTs?	Returns the current events for the pulse table measurement.
STATus:PULSe:STATistics:EVENTs?	Returns the current events for the pulse statistics measurement.
STATus:PULSe:TRACe:EVENTs?	Returns the current events for the pulse trace measurement.
STATus:QUEStionable:CONDition?	Queries the contents of the QCR.
STATus:QUEStionable:ENABle	Sets or queries the mask for the OENR.
STATus:QUEStionable[:EVENT]?	Queries the contents of the QER.
STATus:QUEStionable:NTRansition	Sets or queries the value of the negative transition filter.
STATus:QUEStionable:PTRansition	Sets or queries the value of the positive transition filter.

Table 2-23: Status commands (cont.)

Header	Description
STATUS:QUESTIONABLE:CALibration:CONDition?	Queries the contents of the questionable calibration condition register.
STATUS:QUESTIONABLE:CALibration:ENABLE	Sets or queries the mask for the questionable calibration enable register.
STATUS:QUESTIONABLE:CALibration[:EVENT]?	Queries the contents of the questionable calibration event register.
STATUS:QUESTIONABLE:CALibration:NTRansition	Sets or queries the value of the negative transition filter.
STATUS:QUESTIONABLE:CALibration:PTRansition	Sets or queries the value of the positive transition filter.
STATUS:QUESTIONABLE:FREQuency:CONDition?	Queries the contents of the questionable frequency condition register.
STATUS:QUESTIONABLE:FREQuency:ENABLE	Sets or queries the mask for the questionable frequency enable register.
STATUS:QUESTIONABLE:FREQuency[:EVENT]?	Queries the contents of the questionable frequency event register.
STATUS:QUESTIONABLE:FREQuency:NTRansition	Sets or queries the value of the negative transition filter.
STATUS:QUESTIONABLE:FREQuency:PTRansition	Sets or queries the value of the positive transition filter.
STATUS:SGRAM:EVENTs?	Returns the current events for the spectrogram measurement.
STATUS:SPECTrum:EVENTs?	Returns the current events for the spectrum measurement.
STATUS:SPURious:EVENTs?	Returns the current events for the spurious measurement.
STATUS:SQUality:EVENTs?	Returns the current events for the signal quality measurement.
STATUS:TDIagram:EVENTs?	Returns the current events for the trellis diagram measurement.

System Commands

Use the SYSTem commands to set or query system parameters for operation.

Table 2-24: System commands

Header	Description
SYSTem:COMMunicate:GPIB[:SELF]:ADDRESS	Sets or queries the GPIB address of the instrument.
SYSTem:DATE	Sets or queries the current date.
SYSTem:ERRor:ALL?	Queries all the error or event information.
SYSTem:ERRor:CODE:ALL?	Queries all the error or event codes.
SYSTem:ERRor:CODE[:NEXT]?	Queries the latest error or event information.
SYSTem:ERRor:COUNt?	Queries the number of errors or events.
SYSTem:ERRor[:NEXT]?	Queries the latest error or event information.
SYSTem:OPTions?	Queries optional information.
SYSTem:PRESet	Presets the analyzer.
SYSTem:TIME	Sets or queries the current time.
SYSTem:VERSion?	Queries the version of the SCPI.

Trace Commands

Use the TRACe commands to select trace type and to control trace arithmetic.

Table 2-25: Trace commands

Header	Description
TRACe:{AM FM PM} subgroup	AM/FM/PM measurement
TRACe:{AM FM PM}	Determines whether or not to show the trace.
TRACe:{AM FM PM}:DETection	Sets or queries the display detector, the method to be used for decimating traces to fit the available horizontal space on screen.
TRACe<x>:AVTime:DETection	Sets or queries the display detector.
TRACe:{AM FM PM}:FREeze	Sets or queries whether or not to freeze the trace display.
TRACe:{AM FM PM}:FUNction	Sets or queries the trace function.
TRACe<x>:AVTime subgroup	Amplitude versus Time measurement
TRACe<x>:AVTime	Sets or queries whether or not to show the specified trace.
TRACe<x>:AVTime:AVERAge:COUNT	Sets or queries the number of traces to combine for averaging.
TRACe<x>:AVTime:AVERAge:RESet	Clears the average data and resets the average counter.
TRACe<x>:AVTime:COUNT	Sets or queries the count for the Max or Min Hold trace.
TRACe<x>:AVTime:COUNT:ENABLE	Sets or queries whether or not to enable the count for Max/Min Hold.
TRACe<x>:AVTime:COUNT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
TRACe<x>:AVTime:FREeze	Sets or queries whether or not to freeze the display of the trace.
TRACe<x>:AVTime:FUNction	Sets or queries the trace function.
TRACe<x>:AVTime:LEFToperand	Sets or queries the left operand for the math trace.
TRACe<x>:AVTime:RIGHToperand	Sets or queries the right operand for the math trace.
TRACe<x>:AVTime:SELection	Sets or queries the trace number to display the readout.
TRACe<x>:CCDF subgroup	CCDF measurement
TRACe<x>:CCDF:FREeze	Sets or queries whether or not to freeze the display of the trace.
TRACe<x>:CCDF:SELection	Sets or queries the trace number to display the readout.
TRACe<x>:CCDF:SHOW	Sets or queries whether to show or hide the trace.
TRACe<x>:CCDF:X	Sets or queries the horizontal position of the measurement pointer.
TRACe<x>:CCDF:Y?	Queries the vertical position (CCDF value) of the measurement pointer.
TRACe:CONStellation subgroup (Option 21 only)	Constellation measurement
TRACe:CONStellation:MODE	Sets or queries how to display the constellation trace.
TRACe:DIQVTime subgroup (Option 21 only)	Demodulated I&Q versus Time measurement
TRACe:DIQVTime:ENABLE:I	Sets or queries whether to show or hide the trace I.
TRACe:DIQVTime:ENABLE:Q	Determines whether to show or hide the Q trace.
TRACe:DIQVTime:SELection:I	Selects the I trace.
TRACe:DIQVTime:SELection:Q	Selects the Q trace.
TRACe<x>:DPSA subgroup	DPX spectrum measurement

Table 2-25: Trace commands (cont.)

Header	Description
TRACe<x>:DPSA	Sets or queries whether or not to show the waveform.
TRACe<x>:DPSA:AVERAge:COUnT	Sets or queries the number of traces to combine for averaging.
TRACe<x>:DPSA:COLor:CURVe	Sets or queries the color intensity.
TRACe<x>:DPSA:COLor:INTensity	Sets or queries the color intensity in the DPX spectrum view.
TRACe<x>:DPSA:COLor:SCALe:AUTO	Automatically adjusts the Max and Min color settings to display the broadest range of colors.
TRACe<x>:DPSA:DETEction	Sets or queries the function.
TRACe<x>:DPSA:DOT:PERSiStent	Sets or queries whether to enable or disable the dot persistence.
TRACe<x>:DPSA:DOT:PERSiStent:TYPE	Sets or queries the persistence type.
TRACe<x>:DPSA:DOT:PERSiStent:VARiAbLe	Sets or queries the length of time that data points are displayed.
TRACe<x>:DPSA:FREeze	Sets or queries whether or not to freeze the display of the trace.
TRACe<x>:DPSA:FUNCTion	Sets or queries the trace function for the in the DPX spectrum view.
TRACe<x>:DPSA:LEFToperand	Sets or queries the left operand for the math trace.
TRACe<x>:DPSA:RIGHToperand	Sets or queries the right operand for the math trace.
TRACe<x>:DPSA:SELEct	Sets or queries the trace number to display the readout.
TRACe:EDlagram subgroup (Option 21 only)	Eye diagram
TRACe:EDlagram:ENABle:I	Sets or queries whether to show or hide the trace I.
TRACe:EDlagram:ENABle:Q	Sets or queries whether to show or hide the trace Q.
TRACe:EDlagram:SELEct:I	Selects the I trace.
TRACe:EDlagram:SELEct:Q	Selects the Q trace.
TRACe:FVTime subgroup	Frequency versus Time measurement
TRACe:FVTime	Sets or queries whether or not to show the trace.
TRACe:FVTime:AVERAge:COUnT	Sets or queries the number of traces to combine for averaging.
TRACe:FVTime:COUnT	Sets or queries the count for the Max or Min Hold trace.
TRACe:FVTime:COUnT:ENABle	Sets or queries whether or not to enable the count for Max/Min Hold.
TRACe:FVTime:COUnT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
TRACe<x>:FVTime:DETEction	Enables or queries the type of detection for the specified trace.
TRACe:FVTime:FREeze	Sets or queries whether or not to freeze the display of the trace.
TRACe:FVTime:FUNCTion	Sets or queries the trace function.
TRACe:IQVTime subgroup	RF I&Q versus Time measurement
TRACe:IQVTime:AVERAge:COUnT	Sets or queries the number of traces to combine for averaging.
TRACe:IQVTime:COUnT	Sets or queries the count for the Max or Min Hold trace.
TRACe:IQVTime:COUnT:ENABle	Determines whether to enable or disable the count for the Max or Min Hold trace.
TRACe:IQVTime:DETEction	Sets or queries whether or not to enable the count for Max/Min Hold.
TRACe:IQVTime:COUnT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
TRACe:IQVTime:ENABle:I	Sets or queries whether to show or hide the trace I.

Table 2-25: Trace commands (cont.)

Header	Description
TRACe:IQVTime:ENABle:Q	Sets or queries whether to show or hide the trace Q.
TRACe:IQVTime:FReeze	Sets or queries whether to freeze the IQ traces.
TRACe:IQVTime:FUNCTion	Sets or queries the trace function.
TRACe:IQVTime:SElect:I	Sets or queries whether to choose the I trace.
TRACe:IQVTime:SElect:Q	Sets or queries whether to choose the Q trace.
TRACe:OBWidth subgroup	Occupied Bandwidth measurement
TRACe:OBW:MAXHold	Determines whether to enable or disable the Max Hold trace.
TRACe:PHVTime subgroup	Phase versus Time measurement
TRACe:PHVTime	Sets or queries whether or not to show the trace.
TRACe:PHVTime:AVERage:COUNT	Sets or queries the number of traces to combine for averaging.
TRACe:PHVTime:COUNT	Sets or queries the count for the Max or Min Hold trace.
TRACe:PHVTime:COUNT:ENABle	Sets or queries whether or not to enable the count for Max/Min Hold.
TRACe:PHVTime:COUNT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
TRACe<x>:PHVTime:DETECTion	Sets or queries the display detector.
TRACe:PHVTime:FReeze	Sets or queries whether to freeze the trace.
TRACe:PHVTime:FUNCTion	Sets or queries the trace function.
TRACe:PNOise subgroup (Option 11 only)	Phase noise measurement
TRACe<x>:PNOise:SElect	Selects a trace or queries the currently selected trace.
TRACe<x>:PNOise:SHOW	Sets or queries whether to show or hide the trace.
TRACe<x>:PNOise:SMOothing:COUNT	Sets or queries the number of data points for smoothing the trace.
TRACe<x>:PNOise:SMOothing:ENABle	Sets or queries whether to enable smoothing the specified trace.
TRACe<x>:PNOise:SMOothing:RESet	Restarts the smoothing process.
TRACe:SGRam subgroup	Spectrogram measurement
TRACe:SGRam:DETECTion	Sets or queries the method to be used for decimating traces to fit the on screen.
TRACe:SGRam:FReeze	Sets or queries whether or not to freeze the spectrogram display.
TRACe:SGRam:FUNCTion	Sets or queries the trace function for the spectrogram.
TRACe:SGRam:FUNCTion:TIME	Sets or queries the number of traces to combine for the trace function.
TRACe:SGRam:SElect:LINE	Sets or queries the number of line to send to the spectrum display.
TRACe<x>:SPECTrum subgroup	Spectrum measurement
TRACe<x>:SPECTrum	Sets or queries whether to show or hide the specified trace.
TRACe<x>:SPECTrum:AVERage:COUNT	Sets or queries the number of traces to combine for averaging.
TRACe<x>:SPECTrum:AVERage:RESet	Clears the average data and resets the average counter.
TRACe<x>:SPECTrum:COUNT	Sets or queries the count for the Max or Min Hold trace.
TRACe<x>:SPECTrum:COUNT:ENABle	Sets or queries whether or not to enable the count for Max/Min Hold.
TRACe<x>:SPECTrum:COUNT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
TRACe<x>:SPECTrum:DETECTion	Sets or queries the display detector.

Table 2-25: Trace commands (cont.)

Header	Description
TRACe<x>:SPECtrum:FREeze	Sets or queries whether or not to freeze the display of the trace.
TRACe<x>:SPECtrum:FUNction	Sets or queries the trace function.
TRACe<x>:SPECtrum:LEFToperand	Sets or queries the left operand for the math trace.
TRACe<x>:SPECtrum:RIGHToperand	Sets or queries the right operand for the math trace.
TRACe<x>:SPECtrum:SElect	Sets or queries the trace number to display the readout.
TRACe:SPURious subgroup	Spurious measurement
TRACe:SPURious:COUNT	Sets or queries the count for the Max Hold or Average trace.
TRACe:SPURious:COUNT:ENABLE	Sets or queries whether to enable the count for Max Hold or Average.
TRACe:SPURious:COUNT:RESet	Clears Max Hold or Average data and counter, and restarts the process.
TRACe:SPURious:FREeze	Determines whether or not to freeze the display of the trace.
TRACe:SPURious:FUNction	Sets or queries the trace function.
TRACe:TOVerview subgroup	All measurement
TRACe1:TOVerview	Enables display of or queries the display status of the specified trace.
TRACe1:TOVerview:AVERage:COUNT	Sets or queries the number of traces averaged to generate the specified trace.
TRACe1:TOVerview:COUNT	Enables or queries the count set for the specified trace.
TRACe1:TOVerview:COUNT:ENABLE	Enables or queries the Average count for the specified trace.
TRACe1:TOVerview:COUNT:RESet	Sets or queries whether or not to freeze the display of the trace.
TRACe1:TOVerview:DETection	Enables or queries the type of detection for the specified trace.
TRACe1:TOVerview:FREeze	Enables or queries a halt to acquisition updates for the specified trace.
TRACe1:TOVerview:FUNction	Enables or queries the selected Function for the specified trace.

Trace Mnemonics

Multiple traces can be used in some measurement displays. The traces are specified by the trace specifier TRACe<x> (<x>=1 to 5) which is defined for each measurement display as follows.

Table 2-26: Trace mnemonics

Measurement display	TRACe1	TRACe2	TRACe3	TRACe4	TRACe5
Amplitude versus Time	Trace 1	Trace 2	Math trace	NA	NA
CCDF	Trace 1	Trace 2	Gaussian curve	NA	NA
DPX spectrum	+Peak trace	-Peak trace	Average trace	Math trace	Bitmap trace
Phase noise	Trace 1	Trace 2	NA	NA	NA
Spectrum	Trace 1	Trace 2	Trace 3	Math trace	Spectrogram

NOTE. *Valid traces depend on commands. Refer to each command description.*

Trigger commands

Use the TRIGger commands to set up the trigger system.

Table 2-27: Trigger commands

Header	Description
TRIGger:DPSA:SHOW:FRAMES	Sets or queries whether to trigger each segment in the swept mode.
TRIGger:MASK:NEW	Loads a new frequency mask.
TRIGger:MASK:NEW:AUTO	Draws a new frequency mask automatically.
TRIGger:MASK:OPEN	Opens a trigger mask with a specified file.
TRIGger:MASK:SAVE	Saves the current trigger mask to a specified file.
TRIGger[:SEQUENCE]:ADVANCED:HOLDoff	FIRST Sets or queries the trigger holdoff time.
TRIGger[:SEQUENCE]:ADVANCED:SWEep:MODE	Determines whether or not to trigger each segment in the swept acquisition mode.
TRIGger[:SEQUENCE]:ADVANCED:SWEPT:SEGMENT:ENABLE	Determines whether or not to wait for a trigger for each acquisition in a swept spectrum.
TRIGger[:SEQUENCE]:EVENT:INPut:DDENSITY:AMPLitude	Sets or queries the center vertical level for the density trigger region.
TRIGger[:SEQUENCE]:EVENT:EXTFront:IMPedance	Sets or queries the impedance of the external trigger input (front).
TRIGger[:SEQUENCE]:EVENT:EXTFront:LEVEL	Sets or queries the trigger level at the external trigger input (front).
TRIGger[:SEQUENCE]:EVENT:EXTFront:SLOPe	Sets or queries the trigger slope of the external trigger input (front).
TRIGger[:SEQUENCE]:EVENT:EXTRear:SLOPe	Sets or queries the trigger slope of the external trigger input (rear).
TRIGger[:SEQUENCE]:EVENT:GATed	Sets or queries the logic for the gated trigger input.
TRIGger[:SEQUENCE]:EVENT:INPut:FMASK: BANDwidth BWIDTH[:RESolution]:ACTual?	Sets or queries when the trigger occurs in the frequency mask trigger.
TRIGger[:SEQUENCE]:EVENT:INPut:DDENSITY: AMPLitude:TOLerance	Sets or queries the trigger level for the RF input level trigger.
TRIGger[:SEQUENCE]:EVENT:INPut:RUNT:PULse:HIGH: LEVEL	Sets or queries the trigger slope for the RF input level trigger.
TRIGger[:SEQUENCE]:EVENT:INPut:TDBWidth	Sets or queries the time-domain bandwidth.
TRIGger[:SEQUENCE]:EVENT:INPut:TDBWidth:ACTual?	Queries the actual time-domain bandwidth.
TRIGger[:SEQUENCE]:EVENT:INPut:TDBWidth:STATe	Determines whether to set the time-domain bandwidth automatically.
TRIGger[:SEQUENCE]:EVENT:INPut:TYPE	Sets or queries the trigger type for the source of RF input.
TRIGger[:SEQUENCE]:EVENT:SOURce	Sets or queries the trigger event source.
TRIGger[:SEQUENCE]:FORCed	Sets or queries whether to causes a manual trigger.
TRIGger[:SEQUENCE]:IMMEDIATE	Causes a trigger immediately.
TRIGger[:SEQUENCE]:EVENT:INPut:DDENSITY: FREQUENCY	Sets or queries the center horizontal level for the density trigger region.
TRIGger[:SEQUENCE]:EVENT:INPut:DDENSITY: FREQUENCY:TOLerance	Sets or queries the left and right extensions of the density trigger region from the center horizontal level.
TRIGger[:SEQUENCE]:EVENT:INPut:DDENSITY:THReshold	Sets or queries the DPX Density threshold that defines a trigger event.

Table 2-27: Trigger commands (cont.)

Header	Description
TRIGger[:SEquence]:EVENT:INPut:DDENsity:VIOlation	Sets or queries whether a density value higher or lower than the THReshold value defines a trigger event.
TRIGger[:SEquence]:EVENT:INPut:FMASK: {BANDwidth BWIDth[:RESolution]}	ets or queries the Resolution Bandwidth value to be used in the spectrum view for the frequency mask trigger.
TRIGger[:SEquence]:EVENT:INPut:FMASK: BANDwidth BWIDth[:RESolution]:AUTO	Sets or queries whether to automatically set the Resolution Bandwidth value used in the spectrum view for the frequency mask trigger.
TRIGger[:SEquence]:EVENT:INPut:FMASK:VIOlation	Sets or queries when the analyzer triggers in the frequency mask trigger.
TRIGger[:SEquence]:EVENT:INPut:LEVel	Sets or queries the trigger level for the RF input level trigger.
TRIGger[:SEquence]:EVENT:INPut:RUNT:PULSe	Sets or queries the Runt trigger for a positive or negative going pulse.
TRIGger[:SEquence]:EVENT:INPut:RUNT:PULSe:LOW: LEVel	Sets or queries the lower level (second threshold) to qualify a Runt trigger.
TRIGger[:SEquence]:EVENT:INPut:SLOPe	Sets or queries the trigger slope for the RF input level trigger.
TRIGger[:SEquence]:STATus	Sets or queries the trigger mode (Free Run or Triggered).
TRIGger[:SEquence]:TIME:DELay	Sets or queries the trigger delay time.
TRIGger[:SEquence]:TIME:QUALified	LAST Sets or queries the timing qualification setting for triggers.
TRIGger[:SEquence]:TIME:QUALified:TIME<x>	Sets or queries the trigger mode (Free Run or Triggered).
TRIGger[:SEquence]:ADVanced:HOLDoff:ENABLE	Sets or queries the trigger delay time.
TRIGger[:SEquence]:TIME:POSition	Sets or queries the trigger position.

Unit Commands

Specify fundamental units for measurement.

Table 2-28: Unit commands

Header	Description
UNIT:POWer	Sets or queries the unit of power.

Retrieving Response Message

When receiving a query command from the external controller, the analyzer puts the response message on the Output Queue. This message cannot be retrieved unless you perform retrieval operations through the external controller. (For example, call the IBRD subroutine included in the GPIB software of National Instruments.)

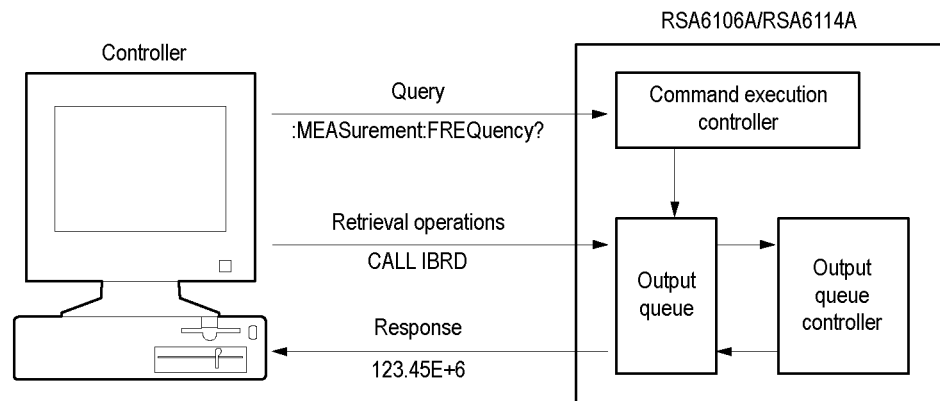


Figure 2-5: Retrieving response message

When the Output Queue contains a response message, sending another command from the external controller before retrieving this message deletes it from the queue. The Output Queue always contains the response message to the most recent query command.

You can use the MAV bit of the Status Byte Register (SBR) to check whether the Output Queue contains a response message. For details, refer to *Status Byte Register (SBR)*.

Command Descriptions

ABORt (No Query Form)

Resets the trigger system and places all trigger sequences in the idle state. Any actions related to the trigger system that are in progress, such as a sweep or acquiring a measurement is also aborted.

To start data acquisition, use the INITiate commands.

Conditions	Measurement views: All
Group	Abort commands
Syntax	ABORt
Related Commands	INITiate:CONTinuous, INITiate[:IMMediate]
Arguments	None
Examples	ABORt resets the trigger system and stops data acquisition.

*CAL (Query Only)

Instructs the analyzer to perform an internal self-alignment and return its status.

NOTE. *The self-alignment can take several minutes to respond. No other commands will be executed until alignment is complete.*

Conditions	Measurement views: All
Group	IEEE common commands
Syntax	*CAL
Returns	<NR1>=1 indicates that the alignment was successful. <NR1>=0 indicates that the alignment was unsuccessful.

Examples *CAL performs an internal self-alignment and will return 1 if the alignment is successful.

CALCulate:ACPower:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker in the Channel power and ACPR measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Channel power and ACPR

Group Calculate commands

Syntax CALCulate:ACPower:MARKer<x>:DELTA:X?

Related Commands [CALCulate:MARKer:ADD](#), [CALCulate:ACPower:MARKer<x>:DELTA:Y?](#)

Returns <NRf> Delta marker frequency for the selected marker.

Examples CALCULATE:ACPOWER:MARKER1:DELTA:X? might return 1.28E+6, indicating that the delta marker frequency is 1.28 MHz.

CALCulate:ACPower:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Channel power and ACPR measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Channel power and ACPR

Group Calculate commands

Syntax CALCulate:ACPower:MARKer<x>:DELTA:Y?

Related Commands [CALCulate:MARKer:ADD](#), [CALCulate:ACPower:MARKer<x>:DELTA:X?](#)

Returns <NRf> Delta marker amplitude for the selected marker.

Examples `CALCULATE:ACPOWER:MARKER1:DELTA:Y?` might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:ACPower:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Calculate commands

Syntax `CALCulate:ACPower:MARKer<x>:MAXimum`

Arguments None

Examples `CALCULATE:ACPOWER:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:ACPower:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Calculate commands

Syntax `CALCulate:ACPower:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:ACPower:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:ACPOWER:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:ACPower:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Calculate commands

Syntax CALCulate:ACPower:MARKer<x>:PEAK:RIGHT

Related Commands [CALCulate:ACPower:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples CALCULATE:ACPOWER:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:ACPower:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Calculate commands

Syntax CALCulate:ACPower:MARKer<x>:X <value>
CALCulate:ACPower:MARKer<x>:X?

Related Commands [CALCulate:ACPower:MARKer<x>:Y?](#)

Arguments `<value> ::= <Nrf>` specifies the horizontal position of the marker.
 Range: Start to Stop frequency (left to right edge of the horizontal axis).
 Using an out-of-range value causes an execution error (-222, "Data out of range").

Examples `CALCULATE:ACPOWER:MARKER1:X 800MHZ` places Marker 1 (M1) at 800 MHz on the trace.

CALCulate:ACPower:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Calculate commands

Syntax `CALCulate:ACPower:MARKer<x>:Y?`

Related Commands [CALCulate:ACPower:MARKer<x>:X](#)

Arguments None

Returns `<Nrf>` Marker amplitude of the selected marker.

Examples `CALCULATE:ACPOWER:MARKER1:Y` might return `-34.28`, indicating Marker 1 (M1) is at -34.28 dBm.

CALCulate:{AM|FM|PM}:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the AM/FM/PM measurement.

The parameter `<x>` = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: General purpose analog demodulation

Group	Calculate commands
Syntax	<code>CALCulate:{AM FM PM}:MARKer<x>:DELTA:X?</code>
Related Commands	CALCulate:{AM FM PM}:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRF> Delta marker time for the selected marker.
Examples	<code>CALCULATE:AM:MARKER1:DELTA:X?</code> might return <code>38.0E-6</code> , indicating that the delta marker time is 38.0 μ s.

CALCulate:{AM|FM|PM}:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the AM/FM/PM measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: General purpose analog demodulation
Group	Calculate commands
Syntax	<code>CALCulate:{AM FM PM}:MARKer<x>:DELTA:Y?</code>
Related Commands	CALCulate:{AM FM PM}:MARKer<x>:DELTA:X?
Arguments	None
Returns	<NRF> Delta marker amplitude for the selected marker, indicating the difference of modulation factor in percent (AM), frequency deviation in Hz (FM), or phase deviation in degrees (PM) with the reference marker.

Examples `CALCULATE:AM:MARKER1:DELTA:Y?` might return `45.82`, indicating that the delta marker amplitude is the modulation factor difference of 45.82% in the AM measurement.

CALCulate:{AM|FM|PM}:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the AM/FM/PM measurement.

Conditions Measurement views: General purpose analog demodulation

Group Calculate commands

Syntax `CALCulate:{AM|FM|PM}:MARKer<x>:MAXimum`

Arguments None

Examples `CALCULATE:AM:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the AM-demodulated trace.

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the trace in the AM/FM/PM measurement.

Conditions Measurement views: General purpose analog demodulation

Group Calculate commands

Syntax `CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:HIGHer`

Related Commands [CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples `CALCULATE:AM:MARKER1:PEAK:HIGHER` moves Marker 1 (M1) to the next peak higher in amplitude on the AM-demodulated trace.

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the AM/FM/PM measurement.

Conditions Measurement views: General purpose analog demodulation

Group Calculate commands

Syntax CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:AM:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the AM-demodulated trace.

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:LOWER (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the trace in the AM/FM/PM measurement.

Conditions Measurement views: General purpose analog demodulation

Group Calculate commands

Syntax CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:LOWER

Related Commands [CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:HIGHER](#)

Arguments None

Examples CALCULATE:AM:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the AM-demodulated trace.

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the AM/FM/PM measurement.

Conditions Measurement views: General purpose analog demodulation

Group Calculate commands

Syntax CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:RIGHT

Related Commands [CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples CALCULATE:AM:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the AM-demodulated trace.

CALCulate:{AM|FM|PM}:MARKer<x>:X

Sets or queries the horizontal position (time) of the selected marker in the AM/FM/PM measurement.

Conditions Measurement views: General purpose analog demodulation

Group Calculate commands

Syntax CALCulate:{AM|FM|PM}:MARKer<x>:X <value>
CALCulate:{AM|FM|PM}:MARKer<x>:X?

Related Commands [CALCulate:{AM|FM|PM}:MARKer<x>:Y?](#)

Arguments <value> ::= <NRf> specifies the horizontal position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Examples CALCULATE:AM:MARKER1:X 1.5us places Marker 1 (M1) at 1.5 μ s on the AM-demodulated trace.

CALCulate:{AM|FM|PM}:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the AM/FM/PM measurement.

Conditions	Measurement views: General purpose analog demodulation
Group	Calculate commands
Syntax	CALCulate:{AM FM PM}:MARKer<x>:Y?
Related Commands	CALCulate:{AM FM PM}:MARKer<x>:X
Arguments	None
Returns	<NRF> Marker amplitude of the selected marker, indicating the modulation factor in percent (AM), frequency deviation in Hz (FM), or phase deviation in degrees (PM) at the marker.
Examples	CALCULATE:AM:MARKER1:Y? might return 23.4, indicating that Marker 1 (M1) reads the modulation factor of 23.4% in the AM measurement.

CALCulate:AVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Amplitude versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Amplitude versus Time
Group	Calculate commands
Syntax	CALCulate:AVTime:MARKer<x>:DELTA:X?
Related Commands	CALCulate:MARKer:ADD , CALCulate:AVTime:MARKer<x>:DELTA:Y?

Returns <NRf> Delta marker time for the selected marker.

Examples CALCULATE:AVTIME:MARKER1:DELTA:X? might return 38.0E-9, indicating that the delta marker time is 38.0 ns.

CALCulate:AVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Amplitude versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax CALCulate:AVTime:MARKer<x>:DELTA:Y?

Related Commands [CALCulate:MARKer:ADD](#), [CALCulate:AVTime:MARKer<x>:DELTA:X?](#)

Returns <NRf> Delta marker amplitude for the selected marker.

Examples CALCULATE:AVTIME:MARKER1:DELTA:Y? might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:AVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Amplitude versus Time measurement.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax CALCulate:AVTime:MARKer<x>:MAXimum

Arguments None

Examples `CALCULATE:AVTIME:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:AVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Amplitude versus Time trace.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax `CALCulate:AVTime:MARKer<x>:PEAK:HIGHer`

Related Commands [CALCulate:AVTime:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples `CALCULATE:AVTIME:MARKER1:PEAK:HIGHER` moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:AVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Amplitude versus Time measurement.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax `CALCulate:AVTime:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:AVTime:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples `CALCulate:AVTime:MARKer1:PEAK:LEFT` moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:AVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Amplitude versus Time trace.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax `CALCulate:AVTime:MARKer<x>:PEAK:LOWer`

Related Commands [CALCulate:AVTime:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples `CALCULATE:AVTIME:MARKER1:PEAK:LOWER` moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:AVTime:MARKer<x>:PEAK:RIGHt (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Amplitude versus Time measurement.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax `CALCulate:AVTime:MARKer<x>:PEAK:RIGHt`

Related Commands [CALCulate:AVTime:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples CALCULATE:AVTIME:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:AVTime:MARKer<x>:TRACe

Sets or queries the trace on which the specified marker is placed in the Amplitude versus Time measurement.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax CALCulate:AVTime:MARKer<x>:TRACe { TRACE1 | TRACE2 | TRACE3 | TRACE4 }
CALCulate:AVTime:MARKer<x>:TRACe?

Arguments TRACE1 places the selected marker on Trace 1.
TRACE2 places the selected marker on Trace 2.
TRACE3 places the selected marker on Trace 3.
TRACE4 places the selected marker on Trace 4 (math trace).

Examples CALCULATE:AVTIME:MARKER1:TRACE TRACE1 places Marker 1 (M1) on Trace 1.

CALCulate:AVTime:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the Amplitude versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax `CALCulate:AVTime:MARKer<x>:X <value>`
`CALCulate:AVTime:MARKer<x>:X?`

Related Commands [CALCulate:AVTime:MARKer<x>:Y?](#)

Arguments `<value> ::= <NRf>` specifies the horizontal position of the marker.
 Range: (analysis offset) to [(analysis offset) + (analysis length)].

Examples `CALCULATE:AVTIME:MARKER1:X 1.5U` places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:AVTime:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Amplitude versus Time measurement.

The parameter `<x>` = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Amplitude versus Time

Group Calculate commands

Syntax `CALCulate:AVTime:MARKer<x>:Y?`

Related Commands [CALCulate:AVTime:MARKer<x>:X](#)

Arguments None

Returns `<NRf>` Marker amplitude of the selected marker.

Examples `CALCULATE:AVTIME:MARKER1:Y?` might return `-2.73`, indicating Marker 1 (M1) is at -2.73 dBm.

CALCulate:CONSte:MARKer<x>:DELTA:X[:TIME]? (Query Only)

Returns the delta marker time for the selected marker on the constellation trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Constellation
Group	Calculate commands
Syntax	<code>CALCulate:CONSte:MARKer<x>:DELTA:X[:TIME]?</code>
Returns	<NRF> Delta marker time for the selected marker. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	<code>CALCULATE:CONSTE:MARKER1:DELTA:X:TIME?</code> might return <code>-62.75</code> , indicating that the delta marker time is -62.75 symbols.

CALCulate:CONSte:MARKer<x>:FDEVIation? (Query Only)

Queries the frequency deviation of the selected marker in the constellation measurement for an FSK modulated signal.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	The command is valid for 2, 4, 8, 16 FSK or C4FM modulated signals.
Group	Calculate commands
Syntax	<code>CALCulate:CONSte:MARKer<x>:FDEVIation?</code>
Related Commands	CALCulate:CONSte:MARKer<x>:MAGNitude? CALCulate:CONSte:MARKer<x>:PHASe?
Arguments	None
Returns	<NRF>The frequency deviation readout for the selected marker.

Examples `CALCulate:CONStE:MARKer1:FDEVIation?` might return `102.824E+3`, indicating the frequency deviation readout of Marker 1 (M1) is 102.824kHz.

CALCulate:CONStE:MARKer<x>:MAGNitude? (Query Only)

Queries the magnitude readout of the selected marker in the constellation measurement.

The parameter `<x>` = 1 to 4; `MARKer0` (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Constellation

Group Calculate commands

Syntax `CALCulate:CONStE:MARKer<x>:MAGNitude?`

Related Commands [CALCulate:CONStE:MARKer<x>:X](#)

Arguments None

Returns `<NRf>` The magnitude readout for the selected marker.

Examples `CALCulate:CONStE:MARKer1:MAGNitude?` might return `0.713927`, indicating the magnitude readout of Marker 1 (M1) is 0.713927.

CALCulate:CONStE:MARKer<x>:MAXimum (No Query Form)

Positions the selected marker at the symbol in the center of the time record.

The parameter `<x>` = 1 to 4; `MARKer0` (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Constellation

Group Calculate commands

Syntax `CALCulate:CONStE:MARKer<x>:MAXimum`

Arguments None

Examples `CALCulate:CONStE:MARKer1:MAXimum` positions Marker 1 (M1) at the symbol in the center of the time record.

CALCulate:CONStE:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker in the time domain to the next lower symbol number, relative to the previous marker position.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Constellation

Group Calculate commands

Syntax `CALCulate:CONStE:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:CONStE:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples `CALCulate:CONStE:MARKer1:PEAK:LEFT` moves Marker 1 (M1) in the time domain to the next lower symbol number.

CALCulate:CONStE:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker in the time domain to the next higher symbol number, relative to the previous marker position.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Constellation

Group	Calculate commands
Syntax	<code>CALCulate:CONStE:MARKer<x>:PEAK:RIGHT</code>
Related Commands	CALCulate:CONStE:MARKer<x>:PEAK:LEFT
Arguments	None
Examples	<code>CALCulate:CONStE:MARKer1:PEAK:RIGHT</code> moves the Marker 1 (M1) in the time domain to the next higher symbol number.

CALCulate:CONStE:MARKer<x>:PHASe? (Query Only)

Queries the phase readout of the selected marker in the constellation measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Constellation
Group	Calculate commands
Syntax	<code>CALCulate:CONStE:MARKer<x>:PHASe?</code>
Related Commands	CALCulate:CONStE:MARKer<x>:X
Arguments	None
Returns	<NRF> The phase readout for the selected marker.
Examples	<code>CALCulate:CONStE:MARKer1:PHASe</code> might return 35.74, indicating the phase readout of Marker 1 (M1) is 35.74 °.

CALCulate:CONSte:MARKer<x>:SYMBol? (Query Only)

Queries the symbol readout of the selected marker in the constellation measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Constellation

Group Calculate commands

Syntax CALCulate:CONSte:MARKer<x>:SYMBol?

Related Commands [CALCulate:CONSte:MARKer<x>:X](#)

Arguments None

Returns <NRF> The symbol readout for the selected marker.

Examples CALCULATE:CONSTE:MARKER1:SYMBOL? might return 62.00, indicating the symbol readout of Marker 1 (M1) is 62.

CALCulate:CONSte:MARKer<x>:VALue? (Query Only)

Queries the value readout of the selected marker in the constellation measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Constellation

Group Calculate commands

Syntax CALCulate:CONSte:MARKer<x>:VALue?

Related Commands [CALCulate:CONSte:MARKer<x>:X](#)

Arguments	None
Returns	<NRf> The value readout for the selected marker.
Examples	CALCULATE:CONSTE:MARKER1:VALUE? might return 2.00, indicating the value readout of Marker 1 (M1) is 2.

CALCulate:CONStE:MARKer<x>:X

Sets or queries the time position of the selected marker on the constellation trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Constellation
Group	Calculate commands
Syntax	CALCulate:CONStE:MARKer<x>:X <value> CALCulate:CONStE:MARKer<x>:X?
Related Commands	CALCulate:CONStE:MARKer<x>:MAGNitude? , CALCulate:CONStE:MARKer<x>:PHASe? , CALCulate:CONStE:MARKer<x>:SYMBol?
Arguments	<value> ::= <NRf> specifies the time position of the marker. Range: (analysis offset) to [(analysis offset) + (analysis length)].
Examples	CALCULATE:CONSTE:MARKER1:X -1.63875m places the Marker 1 (M1) at -1.63875 ms on the constellation trace.

CALCulate:DIQVtime:MARKer<x>:DELTA:X[:TIME]? (Query Only)

Returns the delta marker time for the selected marker on the Demodulated I&Q versus Time trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Demodulated I&Q versus Time
Group	Calculate commands
Syntax	<code>CALCulate:DIQVtime:MARKer<x>:DELTA:X[:TIME]?</code>
Related Commands	CALCulate:DIQVtime:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRF> Delta marker time for the selected marker. Use the [SENSe]:DDEMod:TIME:UNITs command to select the time unit: symbols (default) or seconds.
Examples	<code>CALCULATE:DIQVTIME:MARKER1:DELTA:X:TIME?</code> might return 62.75, indicating that the delta marker time is 62.75 symbols.

CALCulate:DIQVtime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the Demodulated I&Q versus Time trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Demodulated I&Q versus Time
Group	Calculate commands
Syntax	<code>CALCulate:DIQVtime:MARKer<x>:DELTA:Y?</code>
Related Commands	CALCulate:DIQVtime:MARKer<x>:DELTA:X[:TIME]?
Arguments	None
Returns	<NRF> Delta marker amplitude for the selected marker in volts.

Examples `CALCULATE:DIQVTIME:MARKER1:DELTA:Y?` might return `-78.24E-3`, indicating that the delta marker amplitude is -78.24 mV.

CALCulate:DIQVtime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the Demodulated I&Q versus Time trace.

The parameter `<x>` = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax `CALCulate:DIQVtime:MARKer<x>:MAXimum`

Arguments None

Examples `CALCULATE:DIQVTIME:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:DIQVtime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Demodulated I&Q versus Time trace.

The parameter `<x>` = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax `CALCulate:DIQVtime:MARKer<x>:PEAK:HIGHer`

Related Commands [CALCulate:DIQVtime:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples `CALCULATE:DIQVTIME:MARKER1:PEAK:HIGHER` moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:DIQVtime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the Demodulated I&Q versus Time trace.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax `CALCulate:DIQVtime:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:DIQVtime:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples `CALCULATE:DIQVTIME:MARKER1:PEAK:LEFT` moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:DIQVtime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Demodulated I&Q versus Time trace.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax `CALCulate:DIQVtime:MARKer<x>:PEAK:LOWer`

Related Commands [CALCulate:DIQVtime:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples `CALCULATE:DIQVTIME:MARKER1:PEAK:LOWER` moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:DIQVtime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the Demodulated I&Q versus Time trace.

The parameter `<x>` = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax `CALCulate:DIQVtime:MARKer<x>:PEAK:RIGHT`

Related Commands [CALCulate:DIQVtime:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples `CALCULATE:DIQVTIME:MARKER1:PEAK:RIGHT` moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:DIQVtime:MARKer<x>:TRACe

Places the selected marker on the Demodulated I&Q versus Time trace. The query returns the name of the trace on which the marker resides.

The parameter `<x>` = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax CALCulate:DIQVtime:MARKer<x>:TRACe <Enum>
 CALCulate:DIQVtime:MARKer<x>:TRACe?

Related Commands [CALCulate:IQVTime:MARKer<x>:TRACe](#)

Arguments <Enum> ::= TRACE1 | TRACE2 specifies which trace to place the marker on. TRACE1 specifies the “I” trace and TRACE2 specifies the “Q” trace.

Returns For I and Q traces, TRACE1 identifies the “I” trace and TRACE2 identifies the “Q” trace.

Examples CALCulate:DIQVtime:MARKer1:TRACe TRACE1 places Marker 1 (M1) on the I trace.

CALCulate:DIQVtime:MARKer<x>:X[:TIME]

Sets or queries the horizontal position (time) of the selected marker in the Demodulated I&Q versus Time measurement.

The parameter <x> = Marker 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax CALCulate:DIQVtime:MARKer<x>:X[:TIME] <value>
 CALCulate:DIQVtime:MARKer<x>:X[:TIME]?

Related Commands [CALCulate:DIQVtime:MARKer<x>:Y?](#)

Arguments <value> ::= <NRf> specifies the horizontal position (time) of the marker. Use the [\[SENSe\]:DDEMod:TIME:UNITs](#) command to select the time unit: symbols (default) or seconds.

Examples CALCULATE:DIQVTIME:MARKER1:X:TIME 38.5 places Marker 1 (M1) at 38.5 symbols on the trace.

CALCulate:DIQVtime:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Demod I&Q versus Time measurement.

The parameter <x> = Marker 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Demodulated I&Q versus Time

Group Calculate commands

Syntax CALCulate:DIQVtime:MARKer<x>:Y?

Related Commands [CALCulate:DIQVtime:MARKer<x>:X\[:TIME\]](#)

Arguments None

Returns <NRf> Marker amplitude of the selected marker in volts.

Examples CALCulate:DIQVtime:MARKer1:Y? might return 25.803E-3, indicating Marker 1 (M1) is at 25.803 mV.

CALCulate:DPSA:MARKer<x>:DELTA:X:AMPLitude? (Query Only)

Returns the delta marker amplitude for the selected marker on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command and attached to the Bitmap trace using the [CALCulate:DPSA:MARKer<x>:TRACe](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax CALCulate:DPSA:MARKer<x>:DELTA:X:AMPLitude?

Related Commands [CALCulate:DPSA:MARKer<x>:X\[:FREQuency\]](#), [CALCulate:DPSA:MARKer<x>:Y?](#)

Arguments None

Returns <NRF> Delta marker amplitude for the selected marker in dB.

Examples `CALCULATE:DPSA:MARKER1:DELTA:X:AMPLITUDE?` might return `35.12`, indicating that the delta marker amplitude is 35.12 dB for Marker 1 (M1).

CALCulate:DPSA:MARKer<x>:DELTA:X[:FREQuency]? (Query Only)

Returns the delta marker frequency for the selected marker on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax `CALCulate:DPSA:MARKer<x>:DELTA:X[:FREQuency]?`

Related Commands [CALCulate:DPSA:MARKer<x>:DELTA:X:AMPLitude?](#), [CALCulate:DPSA:MARKer<x>:DELTA:Y?](#)

Arguments None

Returns <NRF> Delta marker frequency for the selected marker in Hz.

Examples `CALCULATE:DPSA:MARKER1:DELTA:X?` might return `1.28E+6`, indicating that the delta marker frequency is 1.28 MHz for Marker 1 (M1).

CALCulate:DPSA:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax CALCulate:DPSA:MARKer<x>:DELTA:Y?

Related Commands [CALCulate:DPSA:MARKer<x>:DELTA:X\[:FREQUENCY\]?](#)

Arguments None

Returns <NRf> Delta marker amplitude for the selected marker.

Examples CALCULATE:DPSA:MARKER1:DELTA:Y? might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:DPSA:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax CALCulate:DPSA:MARKer<x>:MAXimum

Arguments None

Examples `CALCULATE:DPSA:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:DPSA:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax `CALCuLate:DPSA:MARKer<x>:PEAK:HIGHer`

Related Commands [CALCulate:DPSA:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples `CALCULATE:DPSA:MARKER1:PEAK:HIGHER` moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:DPSA:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax `CALCuLate:DPSA:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:DPSA:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:DPSA:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:DPSA:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax CALCulate:DPSA:MARKer<x>:PEAK:LOWer

Related Commands [CALCulate:DPSA:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples CALCULATE:DPSA:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:DPSA:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the DPX spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group	Calculate commands
Syntax	<code>CALCulate:DPSA:MARKer<x>:PEAK:RIGHT</code>
Related Commands	CALCulate:DPSA:MARKer<x>:PEAK:LEFT
Arguments	None
Examples	<code>CALCULATE:DPSA:MARKER1:PEAK:RIGHT</code> moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:DPSA:MARKer<x>[:SET]:CENTer (No Query Form)

Sets the center frequency to the marker frequency in the DPX spectrum view.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: DPX spectrum
Group	Calculate commands
Syntax	<code>CALCulate:DPSA:MARKer<x>[:SET]:CENTER</code>
Arguments	None
Examples	<code>CALCULATE:DPSA:MARKER1:SET:CENTER</code> sets the center frequency to the marker frequency in the DPX spectrum view.

CALCulate:DPSA:MARKer<x>:TRACe

Sets or queries the trace to attach the specified marker to in the DPX spectrum measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: DPX spectrum
Group	Calculate commands
Syntax	<code>CALCulate:DPSA:MARKer<x>:TRACe { BITMAP TRACE1 TRACE2 TRACE3 TRACE4 }</code> <code>CALCulate:DPSA:MARKer<x>:TRACe?</code>
Arguments	<p>BITMAP attaches the specified marker to the Bitmap trace.</p> <p>TRACE1 attaches the specified marker to the +Peak trace.</p> <p>TRACE2 attaches the specified marker to the -Peak trace.</p> <p>TRACE3 attaches the specified marker to the Average trace.</p> <p>TRACE4 attaches the specified marker to the Math trace.</p>
Examples	<code>CALCULATE:DPSA:MARKER1:TRACE TRACE1</code> attaches Marker 1 (M1) to the +Peak trace.

CALCulate:DPSA:MARKer<x>:X:AMPLitude

Sets or queries the amplitude position of the selected marker in the DPX spectrum view. This command is valid for the marker on the bitmap trace (refer to the [CALCulate:DPSA:MARKer<x>:TRACe](#) command). The frequency position is set by the [CALCulate:DPSA:MARKer<x>:X:FREQuency](#) command.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: DPX spectrum
Group	Calculate commands
Syntax	<code>CALCulate:DPSA:MARKer<x>:X:AMPLitude <value></code> <code>CALCulate:DPSA:MARKer<x>:X:AMPLitude</code>
Arguments	<code><value> ::= <NRf></code> specifies the amplitude position of the marker. Range: -100 to 0 dBm.

Examples `CALCULATE:DPSA:MARKER1:X:AMPLITUDE -34.5dBm` places Marker 1 (M1) at -34.5 dBm.

CALCulate:DPSA:MARKer<x>:X[:FREQUENCY]

Sets or queries the frequency position of the selected marker in the DPX spectrum view.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group Calculate commands

Syntax `CALCulate:DPSA:MARKer<x>:X[:FREQUENCY] <value>`
`CALCulate:DPSA:MARKer<x>:X[:FREQUENCY]?`

Related Commands [CALCulate:DPSA:MARKer<x>:Y?](#)

Arguments `<value>::=<nrf>` specifies the frequency position of the marker.
Range: Start to Stop frequency (left to right edge of the horizontal axis).
Using an out-of-range value causes an execution error (-222, "Data out of range").

Examples `CALCULATE:DPSA:MARKER1:X:FREQUENCY 800MHZ` places Marker 1 (M1) at 800 MHz on the trace.

CALCulate:DPSA:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the DPX spectrum view. The data occurrence rate is returned for the bitmap trace, and the amplitude value for the +peak, -peak, average, and math traces. The horizontal position can be set by the [CALCulate:DPSA:MARKer<x>:X:AMPLitude](#) and [CALCulate:DPSA:MARKer<x>:X\[:FREQUENCY\]](#) commands.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: DPX spectrum

Group	Calculate commands
Syntax	<code>CALCulate:DPSA:MARKer<x>:Y?</code>
Arguments	None
Returns	<p><Nrf>The value type depends on which trace the marker is placed on (refer to the CALCulate:DPSA:MARKer<x>:TRACe command):</p> <p>The amplitude value is returned in dBm for the marker on the +peak, -peak, average, or math trace. The data occurrence rate is returned in percent (%) for the marker on the bitmap trace.</p>
Examples	<p><code>CALCULATE:DPSA:MARKER1:Y?</code> might return <code>-34.28</code> indicating Marker 1 (M1) is at <code>-34.28</code> dBm when it is placed on the +peak, -peak, average, or math trace.</p> <p><code>CALCULATE:DPSA:MARKER1:Y?</code> might return <code>76.5</code> indicating Marker 1 (M1) is at <code>76.5%</code> when it is placed on the bitmap trace.</p>

`CALCulate:EDIagram:MARKer<x>:DELTA:X[:TIME]? (Query Only)`

Returns the delta marker time for the selected marker on the eye diagram trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Eye diagram
Group	Calculate commands
Syntax	<code>CALCulate:EDIagram:MARKer<x>:DELTA:X[:TIME]?</code>
Related Commands	CALCulate:EDIagram:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<p><Nrf> Delta marker time for the selected marker.</p> <p>Use the [SENSe]:DDEMod:TIME:UNITs command to select the time unit: symbols (default) or seconds.</p>

Examples `CALCulate:EDIagram:MARKer1:DELTA:X:TIME?` might return `62.75`, indicating that the delta marker time is 62.75 symbols.

CALCulate:EDIagram:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the eye diagram trace.

The parameter `<x>` = 1 to 4; `MARKer0` (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax `CALCulate:EDIagram:MARKer<x>:DELTA:Y?`

Related Commands [CALCulate:EDIagram:MARKer<x>:DELTA:X\[:TIME\]?](#)

Arguments None

Returns `<Nrf>` Delta marker amplitude for the selected marker.

Examples `CALCULATE:EDIAGRAM:MARKER1:DELTA:Y?` might return `-1.043`, indicating that the delta marker amplitude is -1.043.

CALCulate:EDIagram:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the eye diagram trace.

The parameter `<x>` = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax `CALCulate:EDIagram:MARKer<x>:MAXimum`

Arguments None

Examples CALCULATE:EDIAGRAM:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:EDIagram:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the eye diagram trace.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax CALCulate:EDIagram:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:EDIagram:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples CALCULATE:EDIAGRAM:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:EDIagram:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the eye diagram trace.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax CALCulate:EDIagram:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:EDIagram:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:EDIAGRAM:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:EDIagram:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the eye diagram trace.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax CALCulate:EDIagram:MARKer<x>:PEAK:LOWer

Related Commands [CALCulate:EDIagram:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples CALCULATE:EDIAGRAM:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:EDIagram:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the eye diagram trace.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax `CALCulate:EDIagram:MARKer<x>:PEAK:RIGHT`

Related Commands [CALCulate:EDIagram:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples `CALCULATE:EDIAGRAM:MARKER1:PEAK:RIGHT` moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:EDIagram:MARKer<x>:TRACe

Places the selected marker on the I or Q trace in the eye diagram display. The query returns the name of the trace on which the marker resides. Valid on all modulation types except 2|4|8|16FSK or C4FM.

The parameter `<x>` = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax `CALCulate:EDIagram:MARKer<x>:TRACe <Enum>`
`CALCulate:EDIagram:MARKer<x>:TRACe?`

Related Commands [CALCulate:EDIagram:MARKer<x>:X\[:TIME\]](#)

Arguments `<Enum> ::= TRACE1 | TRACE2` specifies which trace to place the marker on. TRACE1 specifies the “I” trace and TRACE2 specifies the “Q” trace.

Returns For I and Q traces, TRACE1 identifies the “I” trace and TRACE2 identifies the “Q” trace.

Examples `CALCulate:EDIagram:MARKer1:TRACe TRACE1` places Marker 1 (M1) on the I trace in an eye diagram.

CALCulate:EDIagram:MARKer<x>:X[:TIME]

Sets or queries the horizontal position (time) of the selected marker in the eye diagram measurement.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax CALCulate:EDIagram:MARKer<x>:X[:TIME] <value>
CALCulate:EDIagram:MARKer<x>:X[:TIME]?

Related Commands [CALCulate:EDIagram:MARKer<x>:Y?](#)

Arguments <value>::=<NRf> specifies the horizontal position (time) of the marker. Use the [\[SENSe\]:DDEMod:TIME:UNITs](#) command to select the time unit: symbols (default) or seconds.

Examples CALCulate:EDIagram:MARKer1:X:TIME 38.5 places Marker 1 (M1) at 38.5 symbols on the trace.

CALCulate:EDIagram:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the eye diagram measurement.

The parameter <x> = 0 to 4. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Eye diagram

Group Calculate commands

Syntax CALCulate:EDIagram:MARKer<x>:Y?

Related Commands [CALCulate:EDIagram:MARKer<x>:X\[:TIME\]](#)

Arguments	None
Returns	<Nrf> Vertical position of the selected marker.
Examples	CALCULATE:EDIAGRAM:MARKER1:Y? might return 571.8E-3, indicating Marker 1 (M1) is at 0.5718.

CALCulate:EVM:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the EVM versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: EVM versus Time
Group	Calculate commands
Syntax	CALCulate:EVM:MARKer<x>:DELTA:X?
Related Commands	CALCulate:EVM:MARKer<x>:DELTA:Y?

Arguments	None
Returns	<Nrf> Delta marker time for the selected marker. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	CALCulate:EVM:MARKer1:DELTA:X? might return 9.52, indicating that the delta marker time is 9.52 symbols.

CALCulate:EVM:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the EVM versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: EVM versus Time
Group	Calculate commands
Syntax	CALCulate:EVM:MARKer<x>:DELTA:Y?
Related Commands	CALCulate:EVM:MARKer<x>:DELTA:X?
Arguments	None
Returns	<NRF> Delta marker amplitude for the selected marker in percent (%).
Examples	CALCULATE:EVM:MARKER1:DELTA:Y? might return 1.62, indicating that the delta marker amplitude is 1.62%.

CALCulate:EVM:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the EVM versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: EVM versus Time
Group	Calculate commands
Syntax	CALCulate:EVM:MARKer<x>:MAXimum
Arguments	None

Examples `CALCULATE:EVM:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:EVM:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the EVM versus Time trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: EVM versus Time

Group Calculate commands

Syntax `CALCulate:EVM:MARKer<x>:PEAK:HIGHer`

Related Commands [CALCulate:EVM:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples `CALCULATE:EVM:MARKER1:PEAK:HIGHER` moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:EVM:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the EVM versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: EVM versus Time

Group Calculate commands

Syntax `CALCulate:EVM:MARKer<x>:PEAK:LEFT`

Related Commands	CALCulate:EVM:MARKer<x>:PEAK:RIGHT
Arguments	None
Examples	CALCULATE:EVM:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:EVM:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the EVM versus Time trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: EVM versus Time
Group	Calculate commands
Syntax	CALCulate:EVM:MARKer<x>:PEAK:LOWer

Related Commands	CALCulate:EVM:MARKer<x>:PEAK:HIGHer
Arguments	None
Examples	CALCULATE:EVM:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:EVM:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the EVM versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: EVM versus Time
-------------------	------------------------------------

Group	Calculate commands
Syntax	<code>CALCulate:EVM:MARKer<x>:PEAK:RIGHT</code>
Related Commands	CALCulate:EVM:MARKer<x>:PEAK:LEFT
Arguments	None
Examples	<code>CALCULATE:EVM:MARKER1:PEAK:RIGHT</code> moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:EVM:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the EVM versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: EVM versus Time
Group	Calculate commands
Syntax	<code>CALCulate:EVM:MARKer<x>:X <value></code> <code>CALCulate:EVM:MARKer<x>:X?</code>
Arguments	<value> ::= <NRF> specifies the horizontal position of the marker. Range: (analysis offset) to (analysis offset) + (analysis length). The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	<code>CALCULATE:EVM:MARKER1:X 1.5us</code> places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:EVM:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the EVM versus Time measurement.

Conditions	Measurement views: EVM versus Time
Group	Calculate commands
Syntax	<code>CALCulate:EVM:MARKer<x>:Y?</code>
Related Commands	CALCulate:EVM:MARKer<x>:X
Arguments	None
Returns	<NRF> Marker amplitude of the selected marker in percent (%).
Examples	<code>CALCulate:EVM:MARKer1:Y?</code> might return 5.34, indicating Marker 1 (M1) is at 5.34%.

CALCulate:FDVTime:MARKer<x>:DELTA:X[:TIME]? (Query Only)

Returns the delta marker time for the selected marker on the Frequency deviation vs Time trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Frequency deviation versus Time
Group	Calculate commands
Syntax	<code>CALCulate:FDVTime:MARKer<x>:DELTA:X[:TIME]?</code>
Related Commands	CALCulate:FDVTime:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRF> Delta marker time for the selected marker. Use the [SENSe]:DDEMod:TIME:UNITS command to select the time unit: symbols (default) or seconds.

Examples `CALCULATE:FDVTIME:MARKER1:DELTA:X:TIME?` might return `62.75`, indicating that the delta marker time is 62.75 symbols.

CALCulate:FDVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the Frequency deviation vs Time trace.

The parameter `<x>` = 1 to 4; `MARKer0` (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:DELTA:Y?`

Related Commands [CALCulate:FDVTime:MARKer<x>:DELTA:X\[:TIME\]?](#)

Arguments None

Returns `<NRf>` Delta marker amplitude for the selected marker in Hz.

Examples `CALCULATE:FDVTIME:MARKER1:DELTA:Y?` might return `-563.7E+3`, indicating that the delta marker amplitude is -563.7 kHz.

CALCulate:FDVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the Frequency deviation vs Time trace.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:MAXimum`

Arguments None

Examples `CALCULATE:FDVTIME:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:FDVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Frequency deviation vs Time trace.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:PEAK:HIGHer`

Related Commands [CALCulate:FDVTime:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples `CALCulate:FDVTime:MARKer1:PEAK:HIGHer` moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:FDVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the Frequency deviation vs Time trace.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:FDVTime:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples `CALCULATE:FDVTIME:MARKER1:PEAK:LEFT` moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:FDVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Frequency deviation vs Time trace.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:PEAK:LOWer`

Related Commands [CALCulate:FDVTime:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples `CALCULATE:FDVTIME:MARKER1:PEAK:LOWER` moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:FDVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Frequency deviation versus Time measurement.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:PEAK:RIGHT`

Arguments None

Examples `CALCULATE:FDVTIME:MARKER1:PEAK:RIGHT` moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:FDVTime:MARKer<x>:X[:TIME]

Sets or queries the horizontal position (time) of the selected marker in the Frequency deviation versus Time measurement.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:X[:TIME] <value>`
`CALCulate:FDVTime:MARKer<x>:X[:TIME]?`

Related Commands [CALCulate:FDVTime:MARKer<x>:Y?](#)

Arguments `<value>::=<Nrf>` specifies the horizontal position of the marker.
 Range: (analysis offset) to [(analysis offset) + (analysis length)].
 Use the [\[SENSe\]:DDEMod:TIME:UNITs](#) command to select the time unit: symbols (default) or seconds.

Examples `CALCULATE:FDVTIME:MARKER1:X:TIME 38.5` places Marker 1 (M1) at 38.5 symbols on the trace.

CALCulate:FDVTime:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Frequency deviation versus Time measurement.

Conditions Measurement views: Frequency deviation versus Time

Group Calculate commands

Syntax `CALCulate:FDVTime:MARKer<x>:Y?`

Related Commands [CALCulate:FDVTime:MARKer<x>:X\[:TIME\]](#)

Arguments	None
Returns	<NRf> Marker amplitude of the selected marker in Hz.
Examples	CALCULATE:FDVTIME:MARKER1:Y? might return -15.34E+6, indicating Marker 1 (M1) is at -15.34 MHz.

CALCulate:FVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Frequency versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	CALCulate:FVTime:MARKer<x>:DELTA:X?

Related Commands [CALCulate:FVTime:MARKer<x>:DELTA:Y?](#)

Arguments	None
Returns	<NRf> Delta marker time for the selected marker.
Examples	CALCULATE:FVTIME:MARKER1:DELTA:X? might return 120.0E-9, indicating that the delta marker time is 120 ns.

CALCulate:FVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker frequency for the selected marker in the Frequency versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	<code>CALCulate:FVTime:MARKer<x>:DELTA:Y?</code>
Related Commands	CALCulate:FVTime:MARKer<x>:DELTA:X?
Arguments	None
Returns	<NRF> Delta marker frequency for the selected marker in Hz.
Examples	<code>CALCULATE:FVTIME:MARKER1:DELTA:Y?</code> might return <code>27.05E+3</code> , indicating that the delta marker frequency is 27.05 kHz.

CALCulate:FVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	<code>CALCulate:FVTime:MARKer<x>:MAXimum</code>
Arguments	None
Examples	<code>CALCULATE:FVTIME:MARKER1:MAXIMUM</code> moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:FVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Frequency versus Time trace.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	<code>CALCulate:FVTime:MARKer<x>:PEAK:HIGHer</code>
Related Commands	CALCulate:FVTime:MARKer<x>:PEAK:LOWer
Arguments	None
Examples	<code>CALCULATE:FVTIME:MARKER1:PEAK:HIGHER</code> moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:FVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	<code>CALCulate:FVTime:MARKer<x>:PEAK:LEFT</code>
Related Commands	CALCulate:FVTime:MARKer<x>:PEAK:RIGHT
Arguments	None
Examples	<code>CALCULATE:FVTIME:MARKER1:PEAK:LEFT</code> moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:FVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Frequency versus Time trace.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	<code>CALCulate:FVTime:MARKer<x>:PEAK:LOWer</code>
Related Commands	CALCulate:FVTime:MARKer<x>:PEAK:HIGHer
Arguments	None
Examples	<code>CALCULATE:FVTIME:MARKER1:PEAK:LOWER</code> moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:FVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	<code>CALCulate:FVTime:MARKer<x>:PEAK:RIGHT</code>
Related Commands	CALCulate:FVTime:MARKer<x>:PEAK:LEFT
Arguments	None
Examples	<code>CALCULATE:FVTIME:MARKER1:PEAK:RIGHT</code> moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:FVTime:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	CALCulate:FVTime:MARKer<x>:X <value> CALCulate:FVTime:MARKer<x>:X?
Related Commands	CALCulate:FVTime:MARKer<x>:Y?
Arguments	<value> ::= <Nrf> specifies the horizontal position of the marker. Range: (analysis offset) to [(analysis offset) + (analysis length)].
Examples	CALCULATE:FVTIME:MARKER1:X 1.5u places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:FVTime:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Calculate commands
Syntax	CALCulate:FVTime:MARKer<x>:Y?
Related Commands	CALCulate:FVTime:MARKer<x>:X
Arguments	None
Returns	<Nrf> Marker amplitude of the selected marker in Hz.
Examples	CALCULATE:FVTIME:MARKER1:Y? might return -15.34E+6, indicating Marker 1 (M1) is at -15.34 MHz.

CALCulate:IQVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the RF I&Q versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: RF I&Q versus Time
Group	Calculate commands
Syntax	CALCulate:IQVTime:MARKer<x>:DELTA:X?
Related Commands	CALCulate:IQVTime:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRF> Delta marker time for the selected marker.
Examples	CALCULATE:IQVTIME:MARKER1:DELTA:X? might return 120.0E-9, indicating that the delta marker time is 120 ns.

CALCulate:IQVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the RF I&Q versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: RF I&Q versus Time
Group	Calculate commands
Syntax	CALCulate:IQVTime:MARKer<x>:DELTA:Y?

Related Commands [CALCulate:IQVTime:MARKer<x>:DELTA:X?](#)

Arguments None

Returns <Nrf> Delta marker amplitude for the selected marker in volts.

Examples CALCULATE:IQVTIME:MARKER1:DELTA:Y? might return $-3.45E-3$, indicating that the delta marker amplitude is -3.45 mV.

CALCulate:IQVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Calculate commands

Syntax CALCulate:IQVTime:MARKer<x>:MAXimum

Arguments None

Examples CALCULATE:IQVTIME:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the RF I&Q versus Time trace.

Conditions Measurement views: RF I&Q versus Time

Group Calculate commands

Syntax CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:IQVTime:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples CALCULATE:IQVTIME:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:IQVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Calculate commands

Syntax CALCulate:IQVTime:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:IQVTIME:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:IQVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the RF I&Q versus Time trace.

Conditions Measurement views: RF I&Q versus Time

Group Calculate commands

Syntax CALCulate:IQVTime:MARKer<x>:PEAK:LOWer

Related Commands	CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer
Arguments	None
Examples	CALCULATE:IQVTIME:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the RF I&Q versus Time measurement.

Conditions	Measurement views: RF I&Q versus Time
Group	Calculate commands
Syntax	CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT

Related Commands [CALCulate:IQVTime:MARKer<x>:PEAK:LEFT](#)

Arguments	None
Examples	CALCULATE:IQVTIME:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:IQVTime:MARKer<x>:TRACe

Places the selected marker on the I or Q trace in the RF I&Q versus Time measurement. The query command returns which trace the selected marker is placed on.

Conditions	Measurement views: RF I&Q versus Time
Group	Calculate commands
Syntax	CALCulate:IQVTime:MARKer<x>:TRACe { TRACE1 TRACE2 } CALCulate:IQVTime:MARKer<x>:TRACe?

Arguments TRACE1 places the selected marker on the I trace.
TRACE2 places the selected marker on the Q trace.

Examples CALCULATE:IQVTIME:MARKER1:TRACE TRACE1 places Marker 1 (M1) on the I trace.

CALCulate:IQVTime:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Calculate commands

Syntax CALCulate:IQVTime:MARKer<x>:X <value>
CALCulate:IQVTime:MARKer<x>:X?

Related Commands [CALCulate:IQVTime:MARKer<x>:Y?](#)

Arguments <value>::=<Nrf> specifies the horizontal position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Examples CALCULATE:IQVTIME:MARKER1:X 1.5us places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:IQVTime:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Calculate commands

Syntax CALCulate:IQVTime:MARKer<x>:Y?

Related Commands	CALCulate:IQVTime:MARKer<x>:X
Arguments	None
Returns	<NRf> Marker amplitude of the selected marker in volts.
Examples	CALCULATE:IQVTIME:MARKER1:Y? might return 25.803E-3, indicating Marker 1 (M1) is at 25.803 mV.

CALCulate:MARKer:ADD (No Query Form)

Adds a marker. Every execution of this command adds a marker from MR, then M1 to M4, sequentially.

NOTE. *If all markers are already turned on, the error message "Cannot add another marker" (execution error -200) is returned.*

Conditions	Measurement views: All
Group	Calculate commands
Syntax	CALCulate:MARKer:ADD
Related Commands	CALCulate:MARKer:AOff , CALCulate:MARKer:DELeTe
Arguments	None
Examples	CALCULATE:MARKER:ADD adds a marker.

CALCulate:MARKer:AOff (No Query Form)

Turns off all markers.

Conditions	Measurement views: All
Group	Calculate commands

Syntax CALCulate:MARKer:AOff

Related Commands [CALCulate:MARKer:ADD](#), [CALCulate:MARKer:DELeTe](#)

Arguments None

Examples CALCULATE:MARKER:AOff turns off all markers.

CALCulate:MARKer:DELeTe (No Query Form)

Deletes the last marker added.

NOTE. *If all markers are turned off, the error message "Cannot delete another marker" (execution error -200) is returned.*

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:MARKer:DELeTe

Related Commands [CALCulate:MARKer:ADD](#), [CALCulate:MARKer:AOff](#)

Arguments None

Examples CALCULATE:MARKER:DELETE deletes the last marker added.

CALCulate:MARKer:DENSity:EXCursion

Sets or queries the minimum excursion of DPX signal density, or how far the density (hit count for pixels) must be above the surrounding noise to be detected as a peak. This command is effective for the DPX bitmap trace.

For marker peak up and marker peak down operations, the signal is considered to be a peak if it exceeds the excursion and the threshold set by the CALCulate:MARKer:DENSity:THReshold command.

For marker peak left and marker peak right operations, the signal is considered to be a peak if it first exceeds the amplitude excursion set by `CALCulate:MARKer:PEAK:EXCursion`, the amplitude threshold set by `CALCulate:MARKer:PEAK:THReshold`, the density excursion set by `CALCulate:MARKer:DENSity:EXCursion` and the density threshold set by `CALCulate:MARKer:DENSity:THReshold`.

Conditions Measurement views: All

Group Calculate commands

Syntax `CALCulate:MARKer:DENSity:EXCursion <number>`
`CALCulate:MARKer:DENSity:EXCursion?`

Related Commands [CALCulate:MARKer:DENSity:THReshold](#), [CALCulate:MARKer:PEAK:EXCursion](#), [CALCulate:MARKer:PEAK:THReshold](#)

Arguments `<number>::=<NR1>` specifies the minimum excursion density. Range: 0 to 100%.

Examples `CALCULATE:MARKER:DENSITY:EXCURSION 30` sets the minimum excursion density to 30.

CALCulate:MARKer:DENSity:SMOothing

Sets or queries the number of pixels squared for smoothing the DPX signal density. This command is effective for the DPX bitmap trace.

Conditions Measurement views: All

Group Calculate commands

Syntax `CALCulate:MARKer:DENSity:SMOothing <number>`
`CALCulate:MARKer:DENSity:SMOothing?`

Arguments `<number>::=<NR1>` specifies the number of pixels squared for smoothing the DPX signal density. Range: 1 to 20.

Examples `CALCULATE:MARKER:DENSITY:SMOOTHING 5` sets the smoothing number to 5.

CALCulate:MARKer:DENSity:THReshold

Sets or queries the threshold of DPX signal density above which the density (hit count for pixels) is detected as a peak. This command is effective for the DPX bitmap trace.

Conditions Measurement views: All

Group Calculate commands

Syntax `CALCulate:MARKer:DENSity:THReshold <number>`
`CALCulate:MARKer:DENSity:THReshold?`

Related Commands [CALCulate:MARKer:DENSity:EXCursion](#)

Arguments `<number> ::= <NR1>` specifies the threshold density for detecting peaks.
 Range: 0 to 100%.

Examples `CALCULATE:MARKER:DENSITY:THRESHOLD 300` sets the threshold density to 300.

CALCulate:MARKer:MODE

Sets or queries the marker mode.

Conditions Measurement views: All

Group Calculate commands

Syntax `CALCulate:MARKer:MODE { ABSolute | DELTA }`
`CALCulate:MARKer:MODE?`

Arguments `ABSolute` selects the absolute marker mode, in which the marker readout indicates the absolute value.

DELTA selects the delta marker mode, in which the marker readout indicates the relative value to the reference marker.

Examples CALCULATE:MARKER:MODE DELTA selects the delta marker mode.

CALCulate:MARKer:PEAK:EXCursion

Sets or queries the minimum excursion level (how far a signal must be above the surrounding noise to be detected as a peak). The signal is considered to be a peak if it exceeds the minimum excursion level and the threshold level set by the [CALCulate:MARKer:PEAK:THReshold](#) command.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:MARKer:PEAK:EXCursion <value>
CALCulate:MARKer:PEAK:EXCursion?

Arguments <value>::=<NRF> specifies the excursion level. Range: 0 to 100 dB.

Examples CALCULATE:MARKER:PEAK:EXCURSION 10 sets the excursion level to 10 dB.

CALCulate:MARKer:PEAK:THReshold

Sets or queries the threshold level above which a signal is detected as a peak.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:MARKer:PEAK:THReshold <value>
CALCulate:MARKer:PEAK:THReshold?

Arguments <value>::=<NRF> specifies the threshold level for detecting peaks.
Range: -170 to +130 dBm.

Examples `CALCULATE:MARKER:PEAK:THRESHOLD -50` sets the threshold level to -50 dBm.

CALCulate:MCPower:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker in the MCPR measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: MCPR

Group Calculate commands

Syntax `CALCulate:MCPower:MARKer<x>:DELTA:X?`

Related Commands [CALCulate:MCPower:MARKer<x>:DELTA:Y?](#)

Arguments None

Returns <Nrf> Delta marker frequency for the selected marker.

Examples `CALCULATE:MCPOWER:MARKER1:DELTA:X?` might return `1.28E+6`, indicating that the delta marker frequency is 1.28 MHz.

CALCulate:MCPower:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the MCPR measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: MCPR

Group Calculate commands

Syntax `CALCulate:MCPower:MARKer<x>:DELTA:Y?`

Related Commands `CALCulate:MCPower:MARKer<x>:DELTA:X?`

Arguments None

Returns <NRf> Delta marker amplitude for the selected marker.

Examples `CALCULATE:MCPOWER:MARKER1:DELTA:Y?` might return `23.45`, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:MCPower:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the MCPR measurement.

Conditions Measurement views: MCPR

Group Calculate commands

Syntax `CALCulate:MCPower:MARKer<x>:MAXimum`

Arguments None

Examples `CALCULATE:MCPOWER:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:MCPower:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the MCPR measurement.

Conditions Measurement views: MCPR

Group Calculate commands

Syntax `CALCulate:MCPower:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:MCPower:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples `CALCULATE:MCPOWER:MARKER1:PEAK:LEFT` moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:MCPower:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the MCPR measurement.

Conditions Measurement views: MCPR

Group Calculate commands

Syntax `CALCulate:MCPower:MARKer<x>:PEAK:RIGHT`

Related Commands [CALCulate:MCPower:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples `CALCULATE:MCPOWER:MARKER1:PEAK:RIGHT` moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:MCPower:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the MCPR measurement.

Conditions Measurement views: MCPR

Group Calculate commands

Syntax `CALCulate:MCPower:MARKer<x>:X <value>`
`CALCulate:MCPower:MARKer<x>:X?`

Related Commands [CALCulate:MCPower:MARKer<x>:Y?](#)

Arguments `<value> ::= <Nrf>` specifies the horizontal position of the marker.
 Range: Start to Stop frequency (left to right edge of the horizontal axis).
 Using an out-of-range value causes an execution error (-222, "Data out of range").

Examples `CALCULATE:MCPOWER:MARKER1:X 800MHZ` places Marker 1 (M1) at 800 MHz on the trace.

CALCulate:MCPower:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the MCPR measurement.

Conditions Measurement views: MCPR

Group Calculate commands

Syntax `CALCulate:MCPower:MARKer<x>:Y?`

Related Commands [CALCulate:MCPower:MARKer<x>:X](#)

Arguments None

Returns `<Nrf>` Marker amplitude of the selected marker.

Examples `CALCULATE:MCPOWER:MARKER1:Y?` might return `-34.28`, indicating Marker 1 (M1) is at `-34.28` dBm.

CALCulate:MERRor:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Magnitude error versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Magnitude error versus Time
Group	Calculate commands
Syntax	CALCulate:MERRor:MARKer<x>:DELTA:X?
Related Commands	CALCulate:MERRor:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRf> Delta marker time for the selected marker. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	CALCULATE:MERROR:MARKER1:DELTA:X? might return 9.52, indicating that the delta marker time is 9.52 symbols.

CALCulate:MERRor:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Magnitude error versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Magnitude error versus Time
Group	Calculate commands
Syntax	CALCulate:MERRor:MARKer<x>:DELTA:Y?
Related Commands	CALCulate:MERRor:MARKer<x>:DELTA:X?

Arguments	None
Returns	<Nrf> Delta marker amplitude for the selected marker in percent (%).
Examples	CALCULATE:MERROR:MARKER1:DELTA:Y? might return 3.84, indicating that the delta marker amplitude is 3.84%.

CALCulate:MERRor:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Magnitude error versus Time measurement.

Conditions	Measurement views: Magnitude error versus Time
Group	Calculate commands
Syntax	CALCulate:MERRor:MARKer<x>:MAXimum
Arguments	None
Examples	CALCULATE:MERROR:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:MERRor:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Magnitude error versus Time trace.

Conditions	Measurement views: Magnitude error versus Time
Group	Calculate commands
Syntax	CALCulate:MERRor:MARKer<x>:PEAK:HIGHer
Related Commands	CALCulate:MERRor:MARKer<x>:PEAK:LOWer

Arguments None

Examples CALCULATE:MERROR:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:MERRor:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Calculate commands

Syntax CALCulate:MERRor:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:MERRor:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:MERROR:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:MERRor:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Magnitude error versus Time trace.

Conditions Measurement views: Magnitude error versus Time

Group Calculate commands

Syntax CALCulate:MERRor:MARKer<x>:PEAK:LOWer

Related Commands [CALCulate:MERRor:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples CALCULATE:MERROR:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:MERRor:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Calculate commands

Syntax CALCulate:MERRor:MARKer<x>:PEAK:RIGHT

Related Commands [CALCulate:MERRor:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples CALCULATE:MERROR:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:MERRor:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Calculate commands

Syntax CALCulate:MERRor:MARKer<x>:X <value>
CALCulate:MERRor:MARKer<x>:X?

Arguments <value> ::= <Nrf> specifies the horizontal position of the marker. Range: (analysis offset) to [(analysis offset) + (analysis length)].

The unit can be changed by the [\[SENSE\]:DDEMod:TIME:UNITs](#) command.

Examples `CALCULATE:MERROR:MARKER1:X 1.5u` places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:MERRor:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Calculate commands

Syntax `CALCulate:MERRor:MARKer<x>:Y?`

Related Commands [CALCulate:MERRor:MARKer<x>:X](#)

Arguments None

Returns <NRF> Marker amplitude of the selected marker in percent (%).

Examples `CALCULATE:MERROR:MARKER1:Y?` might return 5.34, indicating Marker 1 (M1) is at 5.34%.

CALCulate:OBWidth:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker in the Occupied Bandwidth measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax `CALCulate:OBWidth:MARKer<x>:DELTA:X?`

Related Commands [CALCulate:OBWidth:MARKer<x>:DELTA:Y?](#)

Arguments None

Returns <Nrf> Delta marker frequency for the selected marker.

Examples `CALCULATE:OBWIDTH:MARKER1:DELTA:X?` might return `1.28E+6`, indicating that the delta marker frequency is 1.28 MHz.

CALCulate:OBWidth:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Occupied Bandwidth measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax `CALCulate:OBWidth:MARKer<x>:DELTA:Y?`

Related Commands [CALCulate:OBWidth:MARKer<x>:DELTA:X?](#)

Arguments None

Returns <Nrf> Delta marker amplitude for the selected marker.

Examples `CALCULATE:OBWIDTH:MARKER1:DELTA:Y?` might return `23.45`, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:OBWidth:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBWidth:MARKer<x>:MAXimum

Arguments None

Examples CALCULATE:OBWIDTH:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Occupied Bandwidth trace.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:OBWidth:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples CALCULATE:OBWIDTH:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:OBWidth:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBWidth:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:OBWIDTH:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:OBWidth:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Occupied Bandwidth trace.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBWidth:MARKer<x>:PEAK:LOWer

Related Commands [CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples CALCULATE:OBWIDTH:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBwidth:MARKer<x>:PEAK:RIGHT

Related Commands [CALCulate:OBWidth:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples CALCULATE:OBWIDTH:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:OBWidth:MARKer<x>[:SET]:CENTER (No Query Form)

Sets the center frequency to the value at the marker position in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBwidth:MARKer<x>[:SET]:CENTER

Arguments None

Examples CALCULATE:OBWIDTH:MARKER1:SET:CENTER sets the center frequency to the value at the Marker 1 position.

CALCulate:OBWidth:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBwidth:MARKer<x>:X <value>
CALCulate:OBwidth:MARKer<x>:X?

Related Commands [CALCulate:OBWidth:MARKer<x>:Y?](#)

Arguments <value> ::= <NRf> specifies the horizontal position of the marker.
Range: Start to Stop frequency (left to right edge of the horizontal axis).
Using an out-of-range value causes an execution error (-222, "Data out of range").

Examples CALCULATE:OBWIDTH:MARKER1:X 800MHZ places Marker 1 (M1) at 800 MHz on the trace.

CALCulate:OBWidth:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Calculate commands

Syntax CALCulate:OBwidth:MARKer<x>:Y?

Related Commands [CALCulate:OBWidth:MARKer<x>:X](#)

Arguments None

Returns <NRf> Marker amplitude of the selected marker.

Examples `CALCULATE:OBWIDTH:MARKER1:Y?` might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

CALCulate:PERRor:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Phase error versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Phase error versus Time

Group Calculate commands

Syntax `CALCulate:PERRor:MARKer<x>:DELTA:X?`

Related Commands [CALCulate:PERRor:MARKer<x>:DELTA:Y?](#)

Arguments None

Returns <NRF> Delta marker time for the selected marker.

The unit can be changed by the [\[SENSe\]:DDEMod:TIME:UNITs](#) command.

Examples `CALCULATE:PERROR:MARKER1:DELTA:X?` might return 9.52, indicating that the delta marker time is 9.52 symbols.

CALCulate:PERRor:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker phase for the selected marker in the Phase error versus Time measurement.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Phase error versus Time

Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:DELTA:Y?</code>
Related Commands	CALCulate:PERRor:MARKer<x>:DELTA:X?
Arguments	None
Returns	<Nrf> Delta marker phase for the selected marker in degrees.
Examples	<code>CALCULATE:PERROR:MARKER1:DELTA:Y?</code> might return <code>-7.93</code> , indicating that the delta marker phase is <code>-7.93 °</code> .

CALCulate:PERRor:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:MAXimum</code>
Arguments	None
Examples	<code>CALCULATE:PERROR:MARKER1:MAXIMUM</code> moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:PERRor:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Phase error versus Time trace.

Conditions	Measurement views: Phase error versus Time
-------------------	--

Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:PEAK:HIGHer</code>
Related Commands	CALCulate:PERRor:MARKer<x>:PEAK:LOWer
Arguments	None
Examples	<code>CALCULATE:PERROR:MARKER1:PEAK:HIGHER</code> moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:PERRor:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:PEAK:LEFT</code>
Related Commands	CALCulate:PERRor:MARKer<x>:PEAK:RIGHT
Arguments	None
Examples	<code>CALCULATE:PERROR:MARKER1:PEAK:LEFT</code> moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:PERRor:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Phase error versus Time trace.

Conditions	Measurement views: Phase error versus Time
-------------------	--

Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:PEAK:LOWer</code>
Related Commands	CALCulate:PERRor:MARKer<x>:PEAK:HIGHer
Arguments	None
Examples	<code>CALCULATE:PERROR:MARKER1:PEAK:LOWER</code> moves Marker 1 (M1) lower in amplitude to the next peak on the trace.

CALCulate:PERRor:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:PEAK:RIGHT</code>
Related Commands	CALCulate:PERRor:MARKer<x>:PEAK:LEFT
Arguments	None
Examples	<code>CALCULATE:PERROR:MARKER1:PEAK:RIGHT</code> moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:PERRor:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
-------------------	--

Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:X <value></code> <code>CALCulate:PERRor:MARKer<x>:X?</code>
Arguments	<code><value>::=<NRF></code> specifies the horizontal position of the marker. Range: (analysis offset) to [(analysis offset) + (analysis length)]. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	<code>CALCULATE:PERRor:MARKer1:X 1.5u</code> places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:PERRor:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Calculate commands
Syntax	<code>CALCulate:PERRor:MARKer<x>:Y?</code>
Related Commands	CALCulate:PERRor:MARKer<x>:X
Arguments	None
Returns	<code><NRF></code> Marker amplitude of the selected marker in degrees.
Examples	<code>CALCULATE:PERRor:MARKer1:Y?</code> might return 21.04, indicating Marker 1 (M1) is at 21.04 $^{\circ}$.

CALCulate:PHVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Phase versus Time measurement.

The parameter $\langle x \rangle = 1$ to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Phase versus Time
Group	Calculate commands
Syntax	CALCulate:PHVTime:MARKer $\langle x \rangle$:DELTA:X?
Related Commands	CALCulate:PHVTime:MARKer$\langle x \rangle$:DELTA:Y?
Arguments	None
Returns	$\langle \text{NRf} \rangle$ Delta marker time for the selected marker.
Examples	CALCULATE:PHVTIME:MARKER1:DELTA:X? might return 38.0E-9, indicating that the delta marker time is 38.0 ns.

CALCulate:PHVTime:MARKer $\langle x \rangle$:DELTA:Y? (Query Only)

Returns the delta marker phase for the selected marker in the Phase versus Time measurement.

The parameter $\langle x \rangle = 1$ to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Phase versus Time
Group	Calculate commands
Syntax	CALCulate:PHVTime:MARKer $\langle x \rangle$:DELTA:Y?
Related Commands	CALCulate:PHVTime:MARKer$\langle x \rangle$:DELTA:X?
Arguments	None

Returns <NRF> Delta marker phase for the selected marker in degrees.

Examples CALCULATE:PHVTIME:MARKER1:DELTA:Y? might return 162.38, indicating that the delta marker phase is 162.38 °.

CALCulate:PHVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Calculate commands

Syntax CALCulate:PHVTime:MARKer<x>:MAXimum

Arguments None

Examples CALCULATE:PHVTIME:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Phase versus Time trace.

Conditions Measurement views: Phase versus Time

Group Calculate commands

Syntax CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:PHVTime:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples `CALCULATE:PHVTIME:MARKER1:PEAK:HIGHER` moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:PHVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Calculate commands

Syntax `CALCulate:PHVTime:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples `CALCULATE:PHVTIME:MARKER1:PEAK:LEFT` moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:PHVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Phase versus Time trace.

Conditions Measurement views: Phase versus Time

Group Calculate commands

Syntax `CALCulate:PHVTime:MARKer<x>:PEAK:LOWer`

Related Commands [CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples `CALCULATE:PHVTIME:MARKER1:PEAK:LOWER` moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Calculate commands

Syntax `CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT`

Related Commands [CALCulate:PHVTime:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples `CALCULATE:PHVTIME:MARKER1:PEAK:RIGHT` moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:PHVTime:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Calculate commands

Syntax `CALCulate:PHVTime:MARKer<x>:X <value>`
`CALCulate:PHVTime:MARKer<x>:X?`

Related Commands [CALCulate:PHVTime:MARKer<x>:Y?](#)

Arguments `<value>::=<NRF>` specifies the horizontal position of the marker.
 Range: (analysis offset) to [(analysis offset) + (analysis length)].

Examples `CALCULATE:PHVTIME:MARKER1:X 1.5US` places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:PHVTime:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Calculate commands

Syntax `CALCulate:PHVTime:MARKer<x>:Y?`

Related Commands [CALCulate:PHVTime:MARKer<x>:X](#)

Arguments None

Returns <NRF> Marker amplitude of the selected marker in degrees.

Examples `CALCULATE:PHVTIME:MARKER1:Y?` might return `-18.435`, indicating Marker 1 (M1) is at `-18.435` $^{\circ}$.

CALCulate:PULSe:STATistics:FFT:INDicator:X

Sets or queries the frequency in Hz for the X indicator. This command is valid when `DISPlay:PULSe:STATistics:PLOT` is set to FFT.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax `CALCulate:PULSe:STATistics:FFT:INDicator:X <value>`
`CALCulate:PULSe:STATistics:FFT:INDicator:X?`

Related Commands [CALCulate:PULSe:STATistics:FFT:INDicator:Y?](#)

Arguments <value>::=<nrf> specifies the indicator X value in Hz.

Examples CALCULATE:PULSE:STATISTICS:FFT:INDICATOR:X 1000 sets the FFT indicator X value to 1 kHz.

CALCulate:PULSe:STATistics:FFT:INDicator:Y? (Query Only)

Returns the frequency level in dB for the Y indicator. This command is valid when DISPLAY:PULSe:STATistics:PLOT is set to FFT.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax CALCulate:PULSe:STATistics:FFT:INDicator:Y?

Related Commands [CALCulate:PULSe:STATistics:FFT:INDicator:X](#)

Returns <nrf> the indicator Y value in dB.

Examples CALCULATE:PULSE:STATISTICS:FFT:INDICATOR:Y? might return -34.5 indicating that the FFT indicator is at -34.5 dB.

CALCulate:PULSe:STATistics:HISTogram:INDicator:X

Sets or queries the histogram indicator X value. This command is valid when DISPLAY:PULSe:STATistics:PLOT is set to histogram.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax CALCulate:PULSe:STATistics:HISTogram:INDicator:X <value>
CALCulate:PULSe:STATistics:HISTogram:INDicator:X?

Related Commands [CALCulate:PULSe:STATistics:HISTogram:INDicator:Y?](#)

Arguments <value>::=<Nrf> specifies the indicator X value.

Examples CALCULATE:PULSE:STATISTICS:HISTOGRAM:INDICATOR:X 0.3 sets the histogram indicator X value to 0.3.

CALCulate:PULSe:STATistics:HISTogram:INDicator:Y? (Query Only)

Queries the Histogram indicator Y value. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to Histogram.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax CALCulate:PULSe:STATistics:HISTogram:INDicator:Y?

Related Commands [CALCulate:PULSe:STATistics:HISTogram:INDicator:X](#)

Returns <Nrf> indicates the indicator Y value.

Examples CALCULATE:PULSE:STATISTICS:HISTOGRAM:INDICATOR:Y? might return 20 to indicate 20 counts in the histogram bin.

CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker on the pulse trace. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to Time Trend.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X?

Related Commands	DISPlay:PULSe:STATistics:PLOT CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y?
Returns	<NRF> Delta marker time in seconds for the selected marker.
Examples	CALCULATE:PULSE:STATISTICS:MARKER1:DELTA:X? might return 3.01e-3, indicating that the delta marker time is 3.01 ms.

CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the pulse trace. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to Time Trend.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Pulse statistics
Group	Calculate commands
Syntax	CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y?
Related Commands	DISPlay:PULSe:STATistics:PLOT CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X?
Returns	<NRF> Delta marker amplitude for the selected marker, in the unit of the current measurement.
Examples	CALCULATE:PULSE:STATISTICS:MARKER1:DELTA:Y? might return 2.345, indicating that the delta marker amplitude is 2.345 dB.

CALCulate:PULSe:STATistics:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the pulse statistics trace. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to Time Trend.

Conditions	Measurement views: Pulse statistics
-------------------	-------------------------------------

Group	Calculate commands
Syntax	<code>CALCulate:PULSE:STATistics:MARKer<x>:MAXimum</code>
Arguments	None
Examples	<code>CALCULATE:PULSE:STATISTICS:MARKER1:MAXIMUM</code> moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:PULSE:STATistics:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the pulse statistics trace. This command is valid when `DISPlay:PULSE:STATistics:PLOT` is set to Time Trend.

Conditions	Measurement views: Pulse statistics
Group	Calculate commands
Syntax	<code>CALCulate:PULSE:STATistics:MARKer<x>:PEAK:HIGHer</code>
Related Commands	CALCulate:PULSE:STATistics:MARKer<x>:PEAK:LOWer
Arguments	None
Examples	<code>CALCULATE:PULSE:STATISTICS:MARKER1:PEAK:HIGHER</code> moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:PULSE:STATistics:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the pulse statistics trace. This command is valid when `DISPlay:PULSE:STATistics:PLOT` is set to Time Trend.

Conditions	Measurement views: Pulse statistics
Group	Calculate commands

Syntax `CALCulate:PULSE:STATISTICS:MARKer<x>:PEAK:LEFT`

Related Commands [CALCulate:PULSE:STATISTICS:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples `CALCULATE:PULSE:STATISTICS:MARKER1:PEAK:LEFT` moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:PULSE:STATISTICS:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the pulse statistics trace. This command is valid when [DISPlay:PULSE:STATISTICS:PLOT](#) is set to Time Trend.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax `CALCulate:PULSE:STATISTICS:MARKer<x>:PEAK:LOWer`

Related Commands [CALCulate:PULSE:STATISTICS:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples `CALCULATE:PULSE:STATISTICS:MARKER1:PEAK:LOWER` moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:PULSE:STATISTICS:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the pulse statistics trace. This command is valid when [DISPlay:PULSE:STATISTICS:PLOT](#) is set to Time Trend.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax `CALCulate:PULSE:STATistics:MARKer<x>:PEAK:RIGHT`

Related Commands [CALCulate:PULSE:STATistics:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples `CALCULATE:PULSE:STATISTICS:MARKER1:PEAK:RIGHT` moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:PULSE:STATistics:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the pulse statistics view. This command is valid when [DISPlay:PULSE:STATistics:PLOT](#) is set to Time Trend.

Conditions Measurement views: Pulse statistics

Group Calculate commands

Syntax `CALCulate:PULSE:STATistics:MARKer<x>:X <value>`
`CALCulate:PULSE:STATistics:MARKer<x>:X?`

Related Commands [CALCulate:PULSE:STATistics:MARKer<x>:Y?](#)

Arguments `<value> ::= <NRf>` specifies the horizontal position of the marker.

Examples `CALCULATE:PULSE:STATISTICS:MARKER1:X 3.01e-3` places Marker 1 (M1) at 3.01 ms on the trace.

CALCulate:PULSE:STATistics:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the pulse statistics view. This command is valid when [DISPlay:PULSE:STATistics:PLOT](#) is set to Time Trend.

Conditions Measurement views: Pulse statistics

Group	Calculate commands
Syntax	CALCulate:PULSE:STATISTICS:MARKer<x>:Y?
Related Commands	CALCulate:PULSE:STATISTICS:MARKer<x>:X
Arguments	None
Returns	<NRF> Amplitude of the specified marker in the unit of the current measurement.
Examples	CALCULATE:PULSE:STATISTICS:MARKER1:Y? might return -28.173, indicating Marker 1 (M1) is at -28.173 dB.

CALCulate:PULSE:TRACe:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker on the pulse trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Pulse trace
Group	Calculate commands
Syntax	CALCulate:PULSE:TRACe:MARKer<x>:DELTA:X?
Related Commands	CALCulate:PULSE:TRACe:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRF>Delta marker time for the selected marker.
Examples	CALCULATE:PULSE:TRACE:MARKER1:DELTA:X? might return 38.0E-9, indicating that the delta marker time is 38.0 ns.

CALCulate:PULSe:TRACe:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the pulse trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:DELTA:Y?

Related Commands [CALCulate:PULSe:TRACe:MARKer<x>:DELTA:X?](#)

Arguments None

Returns <NRf> Delta marker amplitude for the selected marker.

Examples CALCULATE:PULSE:TRACE:MARKER1:DELTA:Y? might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:PULSe:TRACe:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the pulse trace.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:MAXimum

Arguments None

Examples CALCULATE:PULSE:TRACE:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the pulse trace.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples CALCULATE:PULSE:TRACE:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the pulse trace.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:PULSE:TRACE:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the pulse trace.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer

Related Commands [CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples CALCULATE:PULSE:TRACE:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the pulse trace.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT

Related Commands [CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples CALCULATE:PULSE:TRACE:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:PULSe:TRACe:MARKer<x>:X

Sets or queries the horizontal position of the selected marker in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:X <value>
CALCulate:PULSe:TRACe:MARKer<x>:X?

Related Commands [CALCulate:PULSe:TRACe:MARKer<x>:Y?](#)

Arguments <value>::=<NRf> specifies the horizontal position of the marker.

NOTE. To set the horizontal position, the marker must be on the trace of the pulse selected using the [DISPlay:PULSe:SElect:NUMBer](#) command. You cannot put the marker out of the horizontal range of the pulse.

Examples CALCULATE:PULSE:TRACE:MARKER1:X 1.5us places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:PULSe:TRACe:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Calculate commands

Syntax CALCulate:PULSe:TRACe:MARKer<x>:Y?

Related Commands [CALCulate:PULSe:TRACe:MARKer<x>:X](#)

Arguments None

Returns <Nrf> Marker amplitude of the selected marker.

Examples CALCULATE:PULSE:TRACE:MARKER1:Y? might return -28.86, indicating Marker 1 (M1) is at -28.86 dBm.

CALCulate:SEARch:LIMit:FAIL? (Query Only)

Queries whether the waveform cuts across the limit in the search operation.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARch:LIMit:FAIL?

Arguments None

Returns { 0 | 1 }

0 represents Pass, indicating that the waveform does not cut across the limit.

1 represents Fail, indicating that the waveform cuts across the limit.

Examples CALCULATE:SEARCH:LIMIT:FAIL? might return 1, indicating that the waveform cuts across the limit (Fail).

CALCulate:SEARch:LIMit:MATCH:BEEP[:STATe]

Determines whether or not to beep on match during run or replay in the search operation.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARch:LIMit:MATCH:BEEP[:STATe] { OFF | ON | 0 | 1 }
CALCulate:SEARch:LIMit:MATCH:BEEP[:STATe]?

Arguments	OFF or 0 disables to beep on match. ON or 1 enables to beep on match.
Examples	CALCULATE:SEARCH:LIMIT:MATCH:BEEP:STATE ON enables to beep on match.

CALCulate:SEARCh:LIMit:MATCh:SACQuire[:STATe]

Determines whether or not to stop acquiring data on match during run or replay in the search operation.

Conditions	Measurement views: All
Group	Calculate commands
Syntax	CALCulate:SEARCh:LIMit:MATCh:SACQuire[:STATe] { OFF ON 0 1 } CALCulate:SEARCh:LIMit:MATCh:SACQuire[:STATe]?
Arguments	OFF or 0 disables to stop acquiring data on match. ON or 1 enables to stop acquiring data on match.
Examples	CALCULATE:SEARCH:LIMIT:MATCH:SACQUIRE:STATE ON enables to stop acquiring data on match.

CALCulate:SEARCh:LIMit:MATCh:SDATa[:STATe]

Determines whether or not to save automatically (AutoSave) acquisition data on match during run in the search operation.

Conditions	Measurement views: All
Group	Calculate commands
Syntax	CALCulate:SEARCh:LIMit:MATCh:SDATa[:STATe] { OFF ON 0 1 } CALCulate:SEARCh:LIMit:MATCh:SDATa[:STATe]?

- Arguments** OFF or 0 disables the AutoSave.
ON or 1 enables to save acquisition data automatically on match.
The data is saved to a file with the name:
`<name>-yyyy.mm.dd.hh.mm.ss.sss.tiq`
Where
`<name>` is the file name that was last specified.
yyyy.mm.dd and hh.mm.ss.sss represent date and 24 hour time.
The file extension is .tiq.
Example: SAVED-2007.03.20.12.34.567.tiq
For the directory of file, refer to *Specifying the File* (See page 2-47.) in the MMEMory command section.
- Examples** CALCULATE:SEARCH:LIMIT:MATCH:SDATA:STATE ON enables to save acquisition data automatically on match.

CALCulate:SEARCh:LIMit:MATCH:SPICture[:STATE]

Determines whether or not to save automatically (AutoSave) the whole screen on match during run in the search operation.

- Conditions** Measurement views: All
- Group** Calculate commands
- Syntax** CALCulate:SEARCh:LIMit:MATCH:SPICture[:STATE] { OFF | ON | 0 | 1 }
CALCulate:SEARCh:LIMit:MATCH:SPICture[:STATE]?
- Arguments** OFF or 0 disables the AutoSave.
ON or 1 enables to save the whole screen automatically on match.
The picture is saved to a file with the name:
`<name>-yyyy.mm.dd.hh.mm.ss.sss.png`
Where
`<name>` is the file name that was last specified.
yyyy.mm.dd and hh.mm.ss.sss represent date and 24 hour time.
The file extension is .png.
Example: SAVED-2007.03.20.12.34.567.png

For the directory of file, refer to *Specifying the File* (See page 2-47.) in the MMEMory command section.

Examples CALCULATE:SEARCH:LIMIT:MATCH:SPICTURE:STATE ON enables to save the whole screen automatically on match.

CALCulate:SEARCh:LIMit:MATCh:STRace[:STATe]

Determines whether or not to save automatically (AutoSave) the spectrum trace on match during run in the search operation.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARCh:LIMit:MATCh:STRace[:STATe] { OFF | ON | 0 | 1 }
CALCulate:SEARCh:LIMit:MATCh:STRace[:STATe]?

Arguments OFF or 0 disables the AutoSave.
ON or 1 enables to save the spectrum trace automatically on match.
The trace is saved to a file with the name:

<name>-yyyy.mm.dd.hh.mm.ss.sss.Specan

Where

<name> is the file name that was last specified.

yyyy.mm.dd and hh.mm.ss.sss represent date and 24 hour time.

The file extension is .Specan.

Example: SAVED-2007.03.20.12.34.567.Specan

For the directory of file, refer to *Specifying the File* (See page 2-47.) in the MMEMory command section.

Examples CALCULATE:SEARCH:LIMIT:MATCH:STRACE:STATE ON enables to save the spectrum trace automatically on match.

CALCulate:SEARCh:LIMit:OPERation

Sets or queries the search condition.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARCH:LIMit:OPERation { LT | GT | IMASK | OMASK }
CALCulate:SEARCH:LIMit:OPERation?

Related Commands [CALCulate:SEARCh:LIMit:OPERation:SLIMit](#)

Arguments The following table lists the arguments.

Search condition

Argument	Meaning
LT	The data is less than the limit value.
GT	The data is greater than the limit value.
IMASK	The data is inside the limit mask.
OMASK	The data is outside the limit mask.

You can select the data using the [CALCulate:SEARCh:LIMit:OPERation:FEED](#) command.

You can set the limit value using the [CALCulate:SEARCh:LIMit:OPERation:SLIMit](#) command.

You can store and load the limit mask using the [CALCulate:SEARCh:LIMit:OPERation:MASK:STORE](#) and [CALCulate:SEARCh:LIMit:OPERation:MASK:LOAD](#) commands.

Examples CALCULATE:SEARCH:LIMIT:OPERATION GT selects "the data is greater than the limit value" for the search condition.

CALCulate:SEARCh:LIMit:OPERation:FEED

Sets or queries the data flow to be fed in the search operation.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARCH:LIMit:OPERation:FEED <view>,<trace>
 CALCulate:SEARCH:LIMit:OPERation:FEED?

Arguments <view>::=<string> and <trace>::=<string> are listed in the following table.

Source data of the search operation

<view>	<trace>	Meaning
"Spectrum"	"Trace 1" ¹	Trace 1 in the Spectrum view.
	"Trace 2" ¹	Trace 2 in the Spectrum view.
	"Trace 3" ¹	Trace 3 in the Spectrum view.
	"Math Trace"	Math trace in the Spectrum view.
	"Spectrogram Trace"	Spectrogram trace in the Spectrum view.

¹ There is a space character between Trace and the number.

Examples CALCULATE:SEARCH:LIMIT:OPERATION:FEED "Spectrum","Trace 1"
 selects the Trace 1 in the Spectrum measurement view for the search operation.

CALCULATE:SEARCH:LIMIT:OPERATION:FEED? might return
 "Spectrum","Math Trace", indicating that the math trace is used as the source data in the search operation.

CALCulate:SEARch:LIMit:OPERation:MASK:LOAD (No Query Form)

Loads the specified limit mask file for the search operation.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARCH:LIMit:OPERation:MASK:LOAD <file_name>

Arguments <file_name>::=<string> specifies the file to load the limit mask from. The file extension is .lmt. You can omit the extension.

For the directory of file, refer to *Specifying the File* (See page 2-47.) in the MMEMory command section.

Examples CALCULATE:SEARCH:LIMIT:OPERATION:MASK:LOAD "Limit1" loads the limit mask from the *Limit1.lmt* file.

CALCulate:SEARch:LIMit:OPERation:MASK:STORE (No Query Form)

Stores the limit mask to a specified file in the search operation.

Conditions	Measurement views: All
Group	Calculate commands
Syntax	CALCulate:SEARch:LIMit:OPERation:MASK:STORE <file_name>
Arguments	<p><file_name> ::= <string> specifies the file to store the limit mask to. The file extension is .lmt. You can omit the extension.</p> <p>For the directory of file, refer to <i>Specifying the File</i> (See page 2-47.) in the MMEMory command section.</p>
Examples	CALCULATE:SEARCH:LIMIT:OPERATION:MASK:STORE "Limit1" stores the limit mask to the <i>Limit1.lmt</i> file.

CALCulate:SEARch:LIMit:OPERation:SLIMit

Sets or queries the limit value (in dB) in the search operation.

Conditions	Measurement views: All
Group	Calculate commands
Syntax	<p>CALCulate:SEARch:LIMit:OPERation:SLIMit <value></p> <p>CALCulate:SEARch:LIMit:OPERation:SLIMit?</p>
Related Commands	CALCulate:SEARch:LIMit:OPERation
Arguments	<p><value> ::= <Nrf> specifies the limit value in the search operation. Range: -100 to +100 dBm.</p>
Examples	CALCULATE:SEARCH:LIMIT:OPERATION:SLIMIT -20 sets the limit value to -20 dBm.

CALCulate:SEARch:LIMit:REPort:DATA? (Query Only)

Returns the frequency range(s) that satisfy the search condition.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARch:LIMit:REPort:DATA?

Arguments None

Returns <num_range>, <range(1)>, <range(2)>, . . . , <range(n)>

Where

<num_range> ::= <NR1> is the number of ranges that satisfy the condition.

<range(n)> ::= "<lower_freq(n)>, <upper_freq(n)>" (string)

represents the n^{th} frequency range that satisfy the search condition in ascending order. <lower_freq(n)> and <upper_freq(n)> are the lower and upper frequencies of the range #n, respectively.

Examples CALCULATE:SEARCH:LIMIT:REPORT:DATA? might return 2, "1.4800E+9, 1.5001E+9", "1.5002E+9, 1.5200E+9", indicating that the search condition is satisfied in these two ranges 1.48 to 1.5001 GHz and 1.5002 to 1.52 GHz.

CALCulate:SEARch:LIMit:REPort:POINTS? (Query Only)

Returns the number of frequency range(s) that satisfy the search condition.

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARch:LIMit:REPort:POINTS?

Arguments None

Returns <number> ::= <NR1> represents the number of frequency range(s) that satisfy the search condition.

Examples CALCULATE:SEARCH:LIMIT:REPORT:POINTS? might return 5, indicating that five ranges satisfy the search condition.

CALCulate:SEARch:LIMit:STATe

Sets or queries the search function (enabled or disabled).

Conditions Measurement views: All

Group Calculate commands

Syntax CALCulate:SEARch:LIMit:STATe { OFF | ON | 0 | 1 }
CALCulate:SEARch:LIMit:STATe?

Arguments OFF or 0 disables the search function.

ON or 1 enables the search function.

Examples CALCULATE:SEARCH:LIMIT:STATE ON enables the search function.

CALCulate:SGRam:MARKer<x>:DELTA:X:FREQuency? (Query Only)

Returns the delta marker frequency for the selected marker in the spectrogram.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Spectrogram

Group Calculate commands

Syntax CALCulate:SGRam:MARKer<x>:DELTA:X:FREQuency?

Related Commands [CALCulate:SGRam:MARKer<x>:DELTA:Y?](#)

Arguments	None
Returns	<NRF> Delta marker frequency for the selected marker.
Examples	CALCULATE:SGRAM:MARKER1:DELTA:X:FREQUENCY? might return 5.95E+6, indicating that the delta marker frequency is 5.95 MHz.

CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]? (Query Only)

Returns the delta marker time for the selected marker in the spectrogram.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]?
Related Commands	CALCulate:SGRam:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRF> Delta marker time for the selected marker.
Examples	CALCULATE:SGRAM:MARKER1:DELTA:X:TIME? might return -1.84E-3, indicating that the delta marker time is -1.84 ms.

CALCulate:SGRam:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the spectrogram.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	<code>CALCulate:SGRam:MARKer<x>:DELTA:Y?</code>
Related Commands	CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]?
Arguments	None
Returns	<NRf> Delta marker amplitude for the selected marker.
Examples	<code>CALCULATE:SGRAM:MARKER1:DELTA:Y?</code> might return <code>-8.45</code> , indicating that the delta marker amplitude is <code>-8.45</code> dB.

CALCulate:SGRam:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on a line in the spectrogram. The line is selected using the [TRACe:SGRam:SElect:LINE](#) command.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	<code>CALCulate:SGRam:MARKer<x>:MAXimum</code>
Arguments	None
Examples	<code>CALCULATE:SGRAM:MARKER1:MAXIMUM</code> moves Marker 1 (M1) to the highest peak on the line.

CALCulate:SGRam:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on a line in the spectrogram. The line is selected using the [TRACe:SGRam:SElect:LINE](#) command.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	<code>CALCulate:SGRam:MARKer<x>:PEAK:HIGHer</code>
Related Commands	CALCulate:SGRam:MARKer<x>:PEAK:LOWer
Arguments	None
Examples	<code>CALCULATE:SGRAM:MARKER1:PEAK:HIGHER</code> moves Marker 1 (M1) to the next peak higher in amplitude on the line.

CALCulate:SGRam:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on a line in the spectrogram. The line is selected using the [TRACe:SGRam:SElect:LINE](#) command.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	<code>CALCulate:SGRam:MARKer<x>:PEAK:LEFT</code>
Related Commands	CALCulate:SGRam:MARKer<x>:PEAK:RIGHT
Arguments	None
Examples	<code>CALCULATE:SGRAM:MARKER1:PEAK:LEFT</code> moves Marker 1 (M1) to the next peak to the left on the line.

CALCulate:SGRam:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on a line in the spectrogram. The line is selected using the [TRACe:SGRam:SElect:LINE](#) command.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	<code>CALCulate:SGRam:MARKer<x>:PEAK:LOWer</code>
Related Commands	CALCulate:SGRam:MARKer<x>:PEAK:HIGHer
Arguments	None
Examples	<code>CALCULATE:SGRAM:MARKER1:PEAK:LOWER</code> moves Marker 1 (M1) to the next peak lower in amplitude on the line.

CALCulate:SGRam:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on a line in the spectrogram. The line is selected using the [TRACe:SGRam:SElect:LINE](#) command.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	<code>CALCulate:SGRam:MARKer<x>:PEAK:RIGHT</code>
Related Commands	CALCulate:SGRam:MARKer<x>:PEAK:LEFT
Arguments	None
Examples	<code>CALCULATE:SGRAM:MARKER1:PEAK:RIGHT</code> moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:SGRam:MARKer<x>[:SET]:CENTer (No Query Form)

Sets the center frequency to the marker frequency in the spectrogram.

Conditions	Measurement views: Spectrogram
-------------------	--------------------------------

Group	Calculate commands
Syntax	CALCulate:SGRam:MARKer<x>[:SET]:CENTER
Arguments	None
Examples	CALCULATE:SGRAM:MARKER1:SET:CENTER sets the center frequency to the Marker 1 frequency in the spectrogram.

CALCulate:SGRam:MARKer<x>:X:FREQUENCY

Sets or queries the marker frequency in the spectrogram.

Conditions	Measurement views: Spectrogram
Group	Calculate commands
Syntax	CALCulate:SGRam:MARKer<x>:X:FREQUENCY <value> CALCulate:SGRam:MARKer<x>:X:FREQUENCY?
Related Commands	CALCulate:SGRam:MARKer<x>:Y?
Arguments	<value>::=<Nrf> specifies the marker frequency. Range: (center frequency) ± (span)/2.
Examples	CALCULATE:SGRAM:MARKER1:X 800MHZ places Marker 1 (M1) at 800 MHz on the trace.

CALCulate:SGRam:MARKer<x>:X[:TIME]

Sets or queries the marker time in the spectrogram.

Conditions	Measurement views: Spectrogram
Group	Calculate commands

Syntax `CALCulate:SGRam:MARKer<x>:X[:TIME] <value>`
`CALCulate:SGRam:MARKer<x>:X[:TIME]?`

Related Commands [CALCulate:SGRam:MARKer<x>:Y?](#)

Arguments `<value> ::= <NRF>` specifies the marker time.

Examples `CALCULATE:SGRAM:MARKER1:X:TIME -234.5us` places Marker 1 (M1) at -234.5 μ s on the trace.

CALCulate:SGRam:MARKer<x>:Y? (Query Only)

Queries the marker amplitude in the spectrogram.

Conditions Measurement views: Spectrogram

Group Calculate commands

Syntax `CALCulate:SGRam:MARKer<x>:Y?`

Related Commands [CALCulate:SGRam:MARKer<x>:X\[:TIME\]](#)

Arguments None

Returns `<NRF>` Marker amplitude of the selected marker.

Examples `CALCULATE:SGRAM:MARKER1:Y?` might return -34.28, indicating Marker 1 (M1) is at -34.28 dBm.

CALCulate:SPECTrum:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker on the spectrum trace.

The parameter `<x>` = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Spectrum

Group	Calculate commands
Syntax	<code>CALCulate:SPECTrum:MARKer<x>:DELTA:X?</code>
Related Commands	CALCulate:SPECTrum:MARKer<x>:DELTA:Y?
Arguments	None
Returns	<NRF> Delta marker frequency for the selected marker.
Examples	<code>CALCULATE:SPECTRUM:MARKER1:DELTA:X?</code> might return <code>1.28E+6</code> , indicating that the delta marker frequency is 1.28 MHz.

CALCulate:SPECTrum:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Spectrum
Group	Calculate commands
Syntax	<code>CALCulate:SPECTrum:MARKer<x>:DELTA:Y?</code>
Related Commands	CALCulate:SPECTrum:MARKer<x>:DELTA:X?
Arguments	None
Returns	<NRF> Delta marker amplitude for the selected marker.
Examples	<code>CALCULATE:SPECTRUM:MARKER1:DELTA:Y?</code> might return <code>23.45</code> , indicating that the delta marker amplitude is 23.45 dB.

CALCulate:SPECTrum:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the spectrum trace.

Conditions Measurement views: Spectrum

Group Calculate commands

Syntax CALCulate:SPECTrum:MARKer<x>:MAXimum

Arguments None

Examples CALCULATE:SPECTRUM:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the spectrum trace.

Conditions Measurement views: Spectrum

Group Calculate commands

Syntax CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:SPECTrum:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples CALCULATE:SPECTRUM:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the spectrum trace.

Conditions	Measurement views: Spectrum
Group	Calculate commands
Syntax	<code>CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT</code>
Related Commands	CALCulate:SPECTrum:MARKer<x>:PEAK:RIGHT
Arguments	None
Examples	<code>CALCULATE:SPECTRUM:MARKER1:PEAK:LEFT</code> moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:SPECTrum:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the spectrum trace.

Conditions	Measurement views: Spectrum
Group	Calculate commands
Syntax	<code>CALCulate:SPECTrum:MARKer<x>:PEAK:LOWer</code>
Related Commands	CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer
Arguments	None
Examples	<code>CALCULATE:SPECTRUM:MARKER1:PEAK:LOWER</code> moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:SPECTrum:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the spectrum trace.

Conditions	Measurement views: Spectrum
-------------------	-----------------------------

Group	Calculate commands
Syntax	<code>CALCulate:SPECTrum:MARKer<x>:PEAK:RIGHT</code>
Related Commands	CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT
Arguments	None
Examples	<code>CALCULATE:SPECTRUM:MARKER1:PEAK:RIGHT</code> moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:SPECTrum:MARKer<x>[:SET]:CENTER (No Query Form)

Sets the center frequency to the marker frequency in the spectrum measurement.

Conditions	Measurement views: Spectrum
Group	Calculate commands
Syntax	<code>CALCulate:SPECTrum:MARKer<x>[:SET]:CENTER</code>
Arguments	None
Examples	<code>CALCULATE:SPECTRUM:MARKER1:SET:CENTER</code> sets the center frequency to the marker frequency in the spectrum measurement.

CALCulate:SPECTrum:MARKer<x>:TRACe

Sets or queries the trace on which the specified marker is placed in the spectrum measurement.

Conditions	Measurement views: Spectrum
Group	Calculate commands

Syntax `CALCulate:SPECTrum:MARKer<x>:TRACe { TRACE1 | TRACE2 | TRACE3 | TRACE4 | TRACE5 }`
`CALCulate:SPECTrum:MARKer<x>:TRACe?`

Arguments TRACE1 places the specified marker on Trace 1.
TRACE2 places the specified marker on Trace 2.
TRACE3 places the specified marker on n Trace 3.
TRACE4 places the specified marker on Trace 4 (math trace).
TRACE5 places the specified marker on Trace 5 (spectrogram).
Trace 1 to 3 can be defined as Normal, Average, Max Hold or Min Hold using the [TRACE<x>:SPECTrum:FUNCTion](#) command.

Examples `CALCULATE:SPECTRUM:MARKER1:TRACE` TRACE1 places Marker 1 (M1) on Trace 1.

CALCulate:SPECTrum:MARKer<x>:X

Sets or queries the horizontal position of the selected marker on the spectrum trace.

Conditions Measurement views: Spectrum

Group Calculate commands

Syntax `CALCulate:SPECTrum:MARKer<x>:X <value>`
`CALCulate:SPECTrum:MARKer<x>:X?`

Related Commands [CALCulate:SPECTrum:MARKer<x>:Y?](#)

Arguments `<value>::=<NRF>` specifies the horizontal position of the marker.
Range: Start to Stop frequency (left to right edge of the horizontal axis).
Using an out-of-range value causes an execution error (-222, "Data out of range").

Examples `CALCULATE:SPECTRUM:MARKER1:X 800MHZ` places Marker 1 (M1) at 800 MHz on the spectrum trace.

CALCulate:SPECTrum:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker on the spectrum trace.

Conditions Measurement views: Spectrum

Group Calculate commands

Syntax CALCulate:SPECTrum:MARKer<x>:Y?

Related Commands [CALCulate:SPECTrum:MARKer<x>:X](#)

Arguments None

Returns <NRf> Marker amplitude of the selected marker.

Examples CALCULATE:SPECTRUM:MARKER1:Y? might return -34.28, indicating Marker 1 (M1) is at -34.28 dBm.

CALCulate:SPURious:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker on the spectrum trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Spurious

Group Calculate commands

Syntax CALCulate:SPURious:MARKer<x>:DELTA:X?

Arguments None

Returns <NRf> Delta marker frequency for the selected marker.

Examples `CALCULATE:SPURIOUS:MARKER1:DELTA:X?` might return `1.28E+6`, indicating that the delta marker frequency is 1.28 MHz.

CALCulate:SPURious:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the spectrum trace.

The parameter `<x>` = 1 to 4; `MARKer0` (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Spurious

Group Calculate commands

Syntax `CALCulate:SPURious:MARKer<x>:DELTA:Y?`

Arguments None

Returns `<NRf>` Delta marker amplitude for the selected marker.

Examples `CALCULATE:SPURIOUS:MARKER1:DELTA:Y?` might return `23.45`, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:SPURious:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the spectrum trace.

Conditions Measurement views: Spurious

Group Calculate commands

Syntax `CALCulate:SPURious:MARKer<x>:MAXimum`

Arguments None

Examples `CALCULATE:SPURIOUS:MARKER1:MAXIMUM` moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:SPURious:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the spectrum trace.

Conditions Measurement views: Spurious

Group Calculate commands

Syntax `CALCulate:SPURious:MARKer<x>:PEAK:HIGHer`

Arguments None

Examples `CALCULATE:SPURIOUS:MARKER1:PEAK:HIGHER` moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:SPURious:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the spectrum trace.

Conditions Measurement views: Spurious

Group Calculate commands

Syntax `CALCulate:SPURious:MARKer<x>:PEAK:LEFT`

Arguments None

Examples `CALCULATE:SPURIOUS:MARKER1:PEAK:LEFT` moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:SPURious:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the spectrum trace.

Conditions Measurement views: Spurious

Group Calculate commands

Syntax CALCulate:SPURious:MARKer<x>:PEAK:LOWer

Arguments None

Examples CALCULATE:SPURIOUS:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:SPURious:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the spectrum trace.

Conditions Measurement views: Spurious

Group Calculate commands

Syntax CALCulate:SPURious:MARKer<x>:PEAK:RIGHT

Arguments None

Examples CALCULATE:SPURIOUS:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:SPURious:MARKer<x>[:SET]:CENTer (No Query Form)

Sets the center frequency to the marker frequency in the Spurious measurement.

Conditions Measurement views: Spurious

Group	Calculate commands
Syntax	<code>CALCulate:SPURious:MARKer<x>[:SET]:CENTER</code>
Arguments	None
Examples	<code>CALCULATE:SPURIOUS:MARKER1:SET:CENTER</code> sets the center frequency to the value at Marker 1.

CALCulate:SPURious:MARKer<x>:X

Sets or queries the horizontal position of the selected marker on the spectrum trace.

Conditions	Measurement views: Spurious
Group	Calculate commands
Syntax	<code>CALCulate:SPURious:MARKer<x>:X <value></code> <code>CALCulate:SPURious:MARKer<x>:X?</code>
Arguments	<code><value> ::= <NRF></code> specifies the horizontal position of the marker. Range: Start to Stop frequency (left to right edge of the horizontal axis). The start and stop frequencies are set using the DISPlay:SPURious:X[:SCALE]:STARt and DISPlay:SPURious:X[:SCALE]:STOP commands.
Examples	<code>CALCULATE:SPURIOUS:MARKER1:X 800MHZ</code> places Marker 1 (M1) at 800 MHz on the spectrum trace.

CALCulate:SPURious:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker on the spectrum trace.

Conditions	Measurement views: Spurious
Group	Calculate commands

Syntax `CALCulate:SPURious:MARKer<x>:Y?`

Arguments None

Returns <NRF> Marker amplitude of the selected marker.

Examples `CALCULATE:SPURIOUS:MARKER1:Y?` might return `-34.28`, indicating Marker 1 (M1) is at `-34.28` dBm.

CALCulate:TDIagram:MARKer<x>:DELTA:X[:TIME]? (Query Only)

Returns the delta marker time for the selected marker on the Trellis diagram trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Trellis diagram

Group Calculate commands

Syntax `CALCulate:TDIagram:MARKer<x>:DELTA:X[:TIME]?`

Related Commands [CALCulate:TDIagram:MARKer<x>:DELTA:Y?](#)

Arguments None

Returns <NRF> Delta marker time for the selected marker.
Use the [\[SENSe\]:DDEMod:TIME:UNITs](#) command to select the time unit: symbols (default) or seconds.

Examples `CALCULATE:TDIAGRAM:MARKER1:DELTA:X:TIME?` might return `62.75`, indicating that the delta marker time is `62.75` symbols.

CALCulate:TDIagram:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the Trellis diagram trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions	Measurement views: Trellis diagram
Group	Calculate commands
Syntax	CALCulate:TDIagram:MARKer<x>:DELTA:Y?
Related Commands	CALCulate:TDIagram:MARKer<x>:DELTA:X[:TIME]?
Arguments	None
Returns	<NRf> Delta marker amplitude for the selected marker in degrees.
Examples	CALCULATE:TDIAGRAM:MARKER1:DELTA:Y? might return -48.26, indicating that the delta marker amplitude is -48.26°.

CALCulate:TDIagram:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the Trellis diagram trace.

Conditions	Measurement views: Trellis diagram
Group	Calculate commands
Syntax	CALCulate:TDIagram:MARKer<x>:MAXimum
Arguments	None
Examples	CALCULATE:TDIAGRAM:MARKER1:MAXIMUM? moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:TDIagram:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Trellis diagram trace.

Conditions Measurement views: Trellis diagram

Group Calculate commands

Syntax CALCulate:TDIagram:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:TDIagram:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples CALCULATE:TDIAGRAM:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:TDIagram:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the Trellis diagram trace.

Conditions Measurement views: Trellis diagram

Group Calculate commands

Syntax CALCulate:TDIagram:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:TDIagram:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:TDIAGRAM:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:TDIagram:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Trellis diagram trace.

Conditions Measurement views: Trellis diagram

Group Calculate commands

Syntax CALCulate:TDIagram:MARKer<x>:PEAK:LOWer

Related Commands [CALCulate:TDIagram:MARKer<x>:PEAK:HIGHer](#)

Arguments None

Examples CALCULATE:TDIAGRAM:MARKER1:PEAK:LOWER moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:TDIagram:MARKer<x>:PEAK:RIGHt (No Query Form)

Moves the selected marker to the next peak to the right on the Trellis diagram trace.

Conditions Measurement views: Trellis diagram

Group Calculate commands

Syntax CALCulate:TDIagram:MARKer<x>:PEAK:RIGHt

Related Commands [CALCulate:TDIagram:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples CALCULATE:TDIAGRAM:MARKER1:PEAK:RIGHT moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:TDIagram:MARKer<x>:X[:TIME]

Sets or queries the horizontal position (time) of the selected marker in the Trellis diagram measurement.

Conditions Measurement views: Trellis diagram

Group Calculate commands

Syntax CALCulate:TDIagram:MARKer<x>:X[:TIME] <value>
CALCulate:TDIagram:MARKer<x>:X[:TIME]?

Related Commands [CALCulate:TDIagram:MARKer<x>:Y?](#)

Arguments <value> ::= <NRF> specifies the horizontal position (time) of the marker. Use the [\[SENSe\]:DDEMod:TIME:UNITs](#) command to select the time unit: symbols (default) or seconds.

Examples CALCULATE:TDIAGRAM:MARKER1:X:TIME 38.5 places Marker 1 (M1) at 38.5 symbols on the trace.

CALCulate:TDIagram:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the Trellis diagram measurement.

Conditions Measurement views: Trellis diagram

Group Calculate commands

Syntax CALCulate:TDIagram:MARKer<x>:Y?

Related Commands [CALCulate:TDIagram:MARKer<x>:X\[:TIME\]](#)

Arguments None

Returns <NRF> Marker amplitude of the selected marker in degrees.

Examples `CALCULATE:TDIAGRAM:MARKER1:Y?` might return `212.3`, indicating Marker 1 (M1) is at `212.3 °`.

CALCulate:TOVerview:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker on the time overview trace.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax `CALCulate:TOVerview:MARKer<x>:DELTA:X?`

Related Commands [CALCulate:TOVerview:MARKer<x>:DELTA:Y?](#)

Arguments None

Returns <NRf> Delta marker time for the selected marker.

Examples `CALCULATE:TOVERVIEW:MARKER1:DELTA:X?` might return `38.0E-9`, indicating that the delta marker time is `38.0 ns`.

CALCulate:TOVerview:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the time overview trace.

The parameter <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the [CALCulate:MARKer:ADD](#) command.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax `CALCulate:TOVerview:MARKer<x>:DELTA:Y?`

Related Commands [CALCulate:TOVerview:MARKer<x>:DELTA:X?](#)

Arguments None

Returns <NRF> Delta marker amplitude for the selected marker.

Examples CALCULATE:TOVERVIEW:MARKER1:DELTA:Y? might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

CALCulate:TOVerview:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the time overview trace.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax CALCulate:TOVerview:MARKer<x>:MAXimum

Arguments None

Examples CALCULATE:TOVERVIEW:MARKER1:MAXIMUM moves Marker 1 (M1) to the highest peak on the trace.

CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the time overview trace.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer

Related Commands [CALCulate:TOVerview:MARKer<x>:PEAK:LOWer](#)

Arguments None

Examples CALCULATE:TOVIEW:MARKER1:PEAK:HIGHER moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

CALCulate:TOView:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the time overview trace.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax CALCulate:TOView:MARKer<x>:PEAK:LEFT

Related Commands [CALCulate:TOView:MARKer<x>:PEAK:RIGHT](#)

Arguments None

Examples CALCULATE:TOVIEW:MARKER1:PEAK:LEFT moves Marker 1 (M1) to the next peak to the left on the trace.

CALCulate:TOView:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the time overview trace.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax CALCulate:TOView:MARKer<x>:PEAK:LOWer

Related Commands [CALCulate:TOView:MARKer<x>:PEAK:HIGHER](#)

Arguments None

Examples `CALCULATE:TOVERVIEW:MARKER1:PEAK:LOWER` moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

CALCulate:TOVerview:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the time overview trace.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax `CALCulate:TOVerview:MARKer<x>:PEAK:RIGHT`

Related Commands [CALCulate:TOVerview:MARKer<x>:PEAK:LEFT](#)

Arguments None

Examples `CALCULATE:TOVERVIEW:MARKER1:PEAK:RIGHT` moves Marker 1 (M1) to the next peak to the right on the trace.

CALCulate:TOVerview:MARKer<x>:X

Sets or queries the horizontal position of the selected marker on the time overview trace.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax `CALCulate:TOVerview:MARKer<x>:X <value>`
`CALCulate:TOVerview:MARKer<x>:X?`

Related Commands [CALCulate:TOVerview:MARKer<x>:Y?](#)

Arguments `<value>::=<Nrf>` specifies the horizontal position of the marker.
 Range: (analysis offset) to [(analysis offset) + (analysis length)].

Examples `CALCULATE:TOVERVIEW:MARKER1:X 1.5us` places Marker 1 (M1) at 1.5 μ s on the trace.

CALCulate:TOVerview:MARKer<x>:Y? (Query Only)

Queries the marker amplitude of the selected marker in the time overview.

Conditions Measurement views: Time overview

Group Calculate commands

Syntax `CALCulate:TOVerview:MARKer<x>:Y?`

Related Commands [CALCulate:TOVerview:MARKer<x>:X](#)

Arguments None

Returns <NRF> Marker amplitude of the selected marker.

Examples `CALCULATE:TOVERVIEW:MARKER1:Y?` might return `-34.28`, indicating Marker 1 (M1) is at `-34.28` dBm.

CALibration:ABORt (No Query Form)

Aborts any actions related to the alignments in progress.

Conditions Measurement views: All

Group Calibration commands

Syntax `CALibration:ABORt`

Arguments None

Examples `CALIBRATION:ABORT` aborts any actions related to the alignments in progress.

CALibration:AUTO

Sets or queries whether or not to run alignments automatically.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:AUTO { OFF ON 0 1 } CALibration:AUTO?
Arguments	OFF or 0 runs alignments on user request. Use the *CAL command to perform alignments. ON or 1 runs alignments as needed without user intervention. You have to restart measurement if interrupted.
Examples	CALIBRATION:AUTO ON runs alignments automatically as needed.

CALibration:CORRection:EXTErnal:EDIT<x>:LABel

Sets or queries the name of the external loss table.

The parameter <x> = 1 to 3 represent the External Loss Table 1 to 3, respectively.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:CORRection:EXTErnal:EDIT<x>:LABel <name> CALibration:CORRection:EXTErnal:EDIT<x>:LABel?
Arguments	<name>::=<string> specifies the name of the external loss table.
Examples	CALIBRATION:CORRECTION:EXTERNAL:EDIT1:LABEL "Sample Table 1" names the External Loss Table 1 "Sample Table 1".

CALibration:CORRection:EXTErnal:EDIT<x>:NEW (No Query Form)

Creates a new external loss table.

The parameter <x> = 1 to 3 represent the External Loss Table 1 to 3, respectively.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:CORRection:EXTErnal:EDIT<x>:NEW <freq(1)>,<loss(1)>,<freq(2)>,<loss(2)>,...,<freq(n)>,<loss(n)>
Arguments	<freq(n)>,<loss(n)> specifies a pair of frequency (<NR3> in Hz) and loss (<NR3> in dB) in the external loss table. The setting range is: Frequency: 0 to 6.2 GHz (RSA6106A)/14 GHz (RSA6114A) Loss: -50 to +80 dB. (A negative value means a gain.)
Examples	CALIBRATION:CORRECTION:EXTERNAL:EDIT1:NEW 1.0E+9,2.2,1.5E+9,2.3 creates the External Loss Table 1 specifying the loss of 2.2 dB and 2.3 dB at the frequency of 1 GHz and 1.5 GHz, respectively.

CALibration:CORRection:EXTErnal:EDIT<x>:STATE

Determines whether to enable or disable the external loss table.

The parameter <x> = 1 to 3 represent the External Loss Table 1 to 3, respectively.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:CORRection:EXTErnal:EDIT<x>:STATE { OFF ON 0 1 } CALibration:CORRection:EXTErnal:EDIT<x>:STATE?
Arguments	OFF or 0 disables the external loss table. ON or 1 enables the external loss table.

NOTE. *You can enable one or more tables at the same time.*

Examples `CALIBRATION:CORRECTION:EXTERNAL:EDIT3:STATE ON` enables the External Loss Table 3.

CALibration:CORRection:EXTErnal:GAIN[:MAGNitude]

Sets or queries the external gain value. It can be enabled or disabled using the [CALibration:CORRection:EXTErnal:GAIN:STATe](#) command.

Conditions Measurement views: All

Group Calibration commands

Syntax `CALibration:CORRection:EXTErnal:GAIN[:MAGNitude] <value>`
`CALibration:CORRection:EXTErnal:GAIN[:MAGNitude]?`

Arguments `<value> ::= <NRF>` specifies the external gain value. Range: -50 to +30 dB.

Examples `CALIBRATION:CORRECTION:EXTERNAL:GAIN:MAGNITUDE -10` sets the external gain to -10 dB.

CALibration:CORRection:EXTErnal:GAIN:STATe

Determines whether to enable or disable the external gain value.

Conditions Measurement views: All

Group Calibration commands

Syntax `CALibration:CORRection:EXTErnal:GAIN:STATe { OFF | ON | 0 | 1 }`
`CALibration:CORRection:EXTErnal:GAIN:STATe?`

Related Commands [CALibration:CORRection:EXTErnal:GAIN\[:MAGNitude\]](#)

Arguments	OFF or 0 disables the external gain value. ON or 1 enables the external gain value.
Examples	CALIBRATION:CORRECTION:EXTERNAL:GAIN:STATE ON enables the external gain value.

CALibration:CORRection:EXTernal:PROBe:CONNect? (Query Only)

Queries whether the external probe is connected to the analyzer or not.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:CORRection:EXTernal:PROBe:CONNect?
Arguments	None
Returns	{ 0 1 } 0 indicates that the external probe is not connected to the analyzer. 1 indicates that the external probe is connected to the analyzer.
Examples	CALIBRATION:CORRECTION:EXTERNAL:PROBE:CONNECT? might return ON, indicating that the external probe is connected to the analyzer.

CALibration:CORRection:EXTernal:PROBe[:MAGNitude]? (Query Only)

Queries the external probe attenuation.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:CORRection:EXTernal:PROBe[:MAGNitude]?

Arguments	None
Returns	<attenuation>::=<Nrf> The probe attenuation value in dB.
Examples	CALIBRATION:CORRECTION:EXTERNAL:PROBE:MAGNITUDE? might return 10, indicating that the probe attenuation is 10 dB.

CALibration:CORRection:EXTErnal:PROBe:STATe

Determines whether or not to correct data for the external probe attenuation.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:CORRection:EXTErnal:PROBe:STATe { OFF ON 0 1 } CALibration:CORRection:EXTErnal:PROBe:STATe?
Arguments	OFF or 0 does not correct data for the external probe attenuation. ON or 1 corrects data for the external probe attenuation.
Examples	CALIBRATION:CORRECTION:EXTERNAL:PROBE:STATE ON corrects data for the external probe attenuation.

CALibration:CORRection:EXTErnal:TYPE

Sets or queries the data type to apply the external loss table corrections.

Conditions	Measurement views: All
Group	Calibration commands
Syntax	CALibration:CORRection:EXTErnal:TYPE { TRACE DATA } CALibration:CORRection:EXTErnal:TYPE
Related Commands	CALibration:CORRection:EXTErnal:GAIN:STATe

Arguments TRACe selects traces in the Spectrum, Spectrogram, Spurious, and Amplitude versus Time views. Selecting TRACe disables the CALibration:CORRection:EXTErnal:GAIN:STATe command.

DATA selects all acquired data. Selecting DATA enables the CALibration:CORRection:EXTErnal:GAIN:STATe command.

Examples CALIBRATION:CORRECTION:EXTERNAL:TYPE TRACe selects traces to apply the external loss table corrections.

*CLS (No Query Form)

Clears the analyzer status data structures. Refer to Section 3, *Status and Events*, for the register information.

The *CLS command clears the following

- the Event Queue
- the Standard Event Status Register (SESR)
- the Status Byte Register (except the MAV bit; see below)

If the *CLS command immediately follows an <EOI>, the Output Queue and MAV bit (Status Byte Register bit 4) are also cleared. MAV indicates information is in the output queue. The device clear (DCL) GPIB control message will clear the output queue and thus MAV. *CLS does not clear the output queue or MAV. (A complete discussion of these registers and bits, and of event handling in general is described in the *Status and Events* section)

*CLS can suppress a Service Request that is to be generated by an *OPC. This will happen if a hardcopy output or single sequence acquisition operation is still being processed when the *CLS command is executed.

Conditions Measurement views: All

Group IEEE common commands

Syntax *CLS

Related Commands *ESE, *ESR?, *SRE, *STB?

Arguments None

Examples *CLS clears the analyzer status data structures.

DISPlay:ACPower:MARKer:SHOW:STATE

Determines whether to show or hide the readout for the selected marker in the Channel power and ACPR view.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:MARKer:SHOW:STATE { OFF | ON | 0 | 1 }
DISPlay:ACPower:MARKer:SHOW:STATE?

Arguments OFF or 0 hides the readout for the selected marker in the graph.
ON or 1 shows the readout for the selected marker in the graph.

Examples DISPLAY:ACPOWER:MARKER:SHOW:STATE ON shows the readout for the selected marker in the graph.

DISPlay:ACPower:PLEVel:SHOW:STATE

Determines whether to show or hide the power levels in the Channel power and ACPR view.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:PLEVel:SHOW:STATE { OFF | ON | 0 | 1 }
DISPlay:ACPower:PLEVel:SHOW:STATE?

Arguments OFF or 0 hides the power levels in the graph.
ON or 1 shows the power levels in the graph.

Examples DISPLAY:ACPOWER:PLEVEL:SHOW:STATE ON shows the power levels in the graph.

DISPlay:ACPower:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the Channel power and ACPR view.

Vertical offset = Reference level,
Vertical scale = 100 dB,
Horizontal offset = Center frequency, and
Horizontal scale = Default span

Conditions	Measurement views: Channel power and ACPR
Group	Display commands
Syntax	DISP <code>l</code> ay:ACPower:RESet:SCALE
Arguments	None
Examples	DISP <code>l</code> ay:ACPOWER:RESET:SCALE resets the horizontal and vertical scale to the default values.

DISPlay:ACPower:WINDow:TRACe:GRATICule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Channel power and ACPR
Group	Display commands
Syntax	DISP <code>l</code> ay:ACPower:WINDow:TRACe:GRATICule:GRID:STATe { OFF ON 0 1 } DISP <code>l</code> ay:ACPower:WINDow:TRACe:GRATICule:GRID:STATe?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISP <code>l</code> ay:ACPOWER:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen.

DISPlay:ACPower:X[:SCALE]

Sets or queries the horizontal range of the Channel power and ACPR graph.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:X[:SCALE] <value>
DISPlay:ACPower:X[:SCALE]?

Related Commands [DISPlay:ACPower:X\[:SCALE\]:OFFSet](#)

Arguments <value>::=<Nrf> specifies the horizontal range.
Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples DISPLAY:ACPOWER:X:SCALE 10MHZ sets the horizontal range to 10 MHz.

DISPlay:ACPower:X[:SCALE]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the Channel power and ACPR view.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:X[:SCALE]:AUTO

Arguments None

Examples DISPLAY:ACPOWER:X:SCALE:AUTO rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:ACPower:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the Channel power and ACPR graph.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:X[:SCALE]:OFFSet <value>
DISPlay:ACPower:X[:SCALE]:OFFSet?

Related Commands [DISPlay:ACPower:X\[:SCALE\]](#)

Arguments <value>::=<NRF> specifies the minimum horizontal value.
Range: [(center frequency) - (X scale) × 0.9] to [(center frequency) + (X scale) × 0.9]

Examples DISPlay:ACPower:X:SCALE:OFFSet 1.45GHz sets the minimum horizontal value to 1.45 GHz in the Channel power and ACPR graph.

DISPlay:ACPower:Y[:SCALE]

Sets or queries the vertical range of the channel power and ACPR graph.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:Y[:SCALE] <value>
DISPlay:ACPower:Y[:SCALE]?

Related Commands [DISPlay:ACPower:Y\[:SCALE\]:OFFSet](#)

Arguments <value>::=<NRF> specifies the vertical range. Range: 0.1 to 200 dB.

Examples DISPLAY:ACPOWER:Y:SCALE 100 sets the vertical range to 100 dB in the Channel power and ACPR graph.

DISPlay:ACPower:Y[:SCALE]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Channel power and ACPR view.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:Y[:SCALE]:AUTO

Arguments None

Examples DISPLAY:ACPOWER:Y:SCALE:AUTO rescales the vertical scale automatically to fit the waveform to the screen.

DISPlay:ACPower:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the Channel power and ACPR graph.

Conditions Measurement views: Channel power and ACPR

Group Display commands

Syntax DISPlay:ACPower:Y[:SCALE]:OFFSet <value>
DISPlay:ACPower:Y[:SCALE]:OFFSet?

Related Commands [DISPlay:ACPower:Y\[:SCALE\]](#)

Arguments <value>::=<NRF> specifies the vertical offset. Range: -170 to +50 dBm.

Examples DISPLAY:ACPOWER:Y:SCALE:OFFSET -12.5 sets the vertical offset to -12.5 dBm in the Channel power and ACPR graph.

DISPlay:ADEMod:MEASview:DELeTe (No Query Form)

Deletes the measurement view in the general purpose analog demodulation measurements.

Conditions Measurement views: General purpose analog demodulation

Group Display commands

Syntax DISPlay:ADEMod:MEASview:DELeTe { AM | FM | PM }

Arguments The following table lists the arguments.

Table 2-29: Analog demodulation measurement views

Argument	View
AM	AM measurement (modulation factor versus time)
FM	FM measurement (frequency deviation versus time)
PM	PM measurement (phase deviation versus time)

If you attempt to delete a view that is not displayed on screen, the error (-200, "Execution error; Measurement is not running") will be returned.

Examples DISPLAY:ADEMODO:MEASVIEW:DELETE AM deletes the AM measurement view.

DISPlay:ADEMod:MEASview:NEW (No Query Form)

Displays a new measurement view in the general purpose analog demodulation measurements.

Conditions Measurement views: General purpose analog demodulation

Group Display commands

Syntax DISPlay:ADEMod:MEASview:NEW { AM | FM | PM }

Arguments (See Table 2-29 on page 2-227.) If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.

Examples `DISPLAY:AEMOD:MEASVIEW:NEW AM` creates the AM measurement view.

DISPlay:AEMod:MEASview:SElect

Selects a measurement view on the screen in the general purpose analog demodulation measurements. The query command returns the currently selected view.

Selecting a measurement optimizes it. Other measurements may be optimized as a side effect. Refer to the [DISPlay:WINDow:OPTimized:MEASurement?](#) query.

Conditions Measurement views: General purpose analog demodulation

Group Display commands

Syntax `DISPlay:AEMod:MEASview:SElect { AM | FM | PM }`
`DISPlay:AEMod:MEASview:SElect?`

Arguments (See Table 2-29 on page 2-227.) If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Examples `DISPLAY:AEMOD:MEASVIEW:SELECT AM` selects the AM measurement view.

DISPlay:{AM|FM|PM}:MARKer:SHOW:STATe

Determines whether to show or hide the marker readout in the AM/FM/PM measurement view.

Conditions Measurement views: General purpose analog demodulation

Group Display commands

Syntax `DISPlay:{AM|FM|PM}:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }`
`DISPlay:{AM|FM|PM}:MARKer:SHOW:STATe?`

Arguments OFF or 0 hides the marker readout on the screen.

ON or 1 shows the marker readout on the screen.

Examples `DISPLAY:AM:MARKER:SHOW:STATE ON` shows the marker readout in the AM measurement view.

DISPlay:{AM|FM|PM}:WINDow:TRACe:GRATicule:GRID:STATE

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: General purpose analog demodulation

Group Display commands

Syntax `DISPlay:{AM|FM|PM}:WINDow:TRACe:GRATicule:GRID:STATE { OFF | ON | 0 | 1 }`
`DISPlay:{AM|FM|PM}:WINDow:TRACe:GRATicule:GRID:STATE?`

Arguments OFF or 0 hides the graticule grid.

ON or 1 shows the graticule grid.

Examples `DISPLAY:AM:WINDOW:TRACE:GRATICULE:GRID:STATE ON` shows the graticule grid on the AM measurement view.

DISPlay:{AM|FM|PM}:X:RSCale (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the AM/FM/PM measurement display.

Conditions Measurement views: General purpose analog demodulation

Group Display commands

Syntax `DISPlay:{AM|FM|PM}:X:RSCale`

Arguments None

Examples `DISPLAY:AM:X:RSCALE` rescales the horizontal scale automatically to fit the waveform to the screen.

DISP_{lay}:{AM|FM|PM}:X[:SCALE]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the AM/FM/PM measurement display.

Conditions	Measurement views: General purpose analog demodulation
Group	Display commands
Syntax	DISP _{lay} :{AM FM PM}:X[:SCALE]:AUTO
Arguments	None
Examples	DISP _{lay} :AM:X:SCALE:AUTO sets the horizontal scale automatically to fit the waveform to the screen in the AM/FM/PM measurement display.

DISP_{lay}:{AM|FM|PM}:X[:SCALE]:FULL

Sets or queries the horizontal scale (full-scale time) of the AM/FM/PM measurement graph.

Conditions	Measurement views: General purpose analog demodulation
Group	Display commands
Syntax	DISP _{lay} :{AM FM PM}:X[:SCALE]:FULL <value> DISP _{lay} :{AM FM PM}:X[:SCALE]:FULL?
Arguments	<value>::=<Nrf> specifies the horizontal scale in full-scale time. Range: 0 to 10 ²⁷ s.
Examples	DISP _{lay} :AM:X:SCALE:FULL 35us sets the horizontal scale to 35 μs in the AM measurement.

DISP_{lay}:{AM|FM|PM}:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the AM/FM/PM measurement graph.

Conditions	Measurement views: General purpose analog demodulation
Group	Display commands
Syntax	DISPlay:{AM FM PM}:X[:SCALE]:OFFSet <value> DISPlay:{AM FM PM}:X[:SCALE]:OFFSet?
Arguments	<value>::=<NRf> specifies the minimum horizontal value. Range: $-0.9 \times (\text{horizontal scale})$ to $+0.9 \times (\text{horizontal scale})$
Examples	DISPLAY:AM:X:SCALE:OFFSET 20.075us sets the minimum horizontal value to 20.075 μ s.

DISPlay:{AM|FM|PM}:Y:RSCale (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the AM/FM/PM measurement display.

Conditions	Measurement views: General purpose analog demodulation
Group	Display commands
Syntax	DISPlay:{AM FM PM}:Y:RSCale
Arguments	None
Examples	DISPLAY:AM:Y:RSCALE rescales the vertical scale automatically to fit the waveform to the screen in the AM measurement.

DISPlay:{AM|FM|PM}:Y[:SCALE]

Sets or queries the vertical range of the AM/FM/PM measurement graph.

Conditions	Measurement views: General purpose analog demodulation
Group	Display commands

Syntax `DISPlay:{AM|FM|PM}:Y[:SCALE] <value>`
`DISPlay:{AM|FM|PM}:Y[:SCALE]?`

Arguments `<value>::=<Nrf>` specifies the vertical range.
 The setting range depends on measurements as shown in the following table.

Setting range

Measurement	Setting range
AM	1% to 500%
FM	10 Hz to 120 MHz
PM	10° to 400°

Examples `DISPLAY:AM:Y:SCALE 75` sets the vertical range to 75% in the AM measurement graph.

DISPly:{AM|FM|PM}:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (center point of the vertical axis) in the AM/FM/PM measurement graph.

Conditions Measurement views: General purpose analog demodulation

Group Display commands

Syntax `DISPly:{AM|FM|PM}:Y[:SCALE]:OFFSet <value>`
`DISPly:{AM|FM|PM}:Y[:SCALE]:OFFSet?`

Arguments `<value>::=<Nrf>` specifies the vertical offset.
 The setting range depends on measurements as shown in the following table.

Setting range

Measurement	Setting range
AM	-500% to +500%
FM	$-(\text{maxVertScale} * (1 + 1.1) * 0.5)$ to $+(\text{maxVertScale} * (1 + 1.1) * 0.5)$
PM	-180° to +180°

Examples `DISPLAY:AM:Y:SCALE:OFFSET -12.5` sets the vertical offset to -12.5% in the AM measurement graph.

DISPlay:AVTime:LEGend:STATe

Determines whether to show or hide the trace legend in the amplitude versus time view. The legend indicates the trace detection and function on the screen for each displayed trace.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax DISPlay:AVTime:LEGend:STATe { OFF | ON | 0 | 1 }
DISPlay:AVTime:LEGend:STATe?

Arguments OFF or 0 hides the trace legend.
ON or 1 shows the trace legend.

Examples DISPLAY:AVTIME:LEGEND:STATE ON shows the trace legend on the screen.

DISPlay:AVTime:MARKer:SHOW:STATe

Determines whether to show or hide the readout for the selected marker on the screen in the Amplitude versus Time measurement.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax DISPlay:AVTime:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
DISPlay:AVTime:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the readout for the selected marker on screen.
ON or 1 shows the readout for the selected marker on screen.

Examples DISPLAY:AVTIME:MARKER:SHOW:STATE ON shows the readout for the selected marker on screen.

DISPlay:AVTime:RESet (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the Amplitude versus Time view.

Vertical offset = Reference level,
Vertical scale = 100 dB,
Horizontal offset = Analysis offset, and
Horizontal scale = Analysis length

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:RESet
Arguments	None
Examples	DISPLAY:AVTIME:RESET resets the horizontal and vertical scale to the default values.

DISPlay:AVTime:TRIGger:LEVel:STATe

Determines whether to show or hide the power trigger level line on the screen in the Amplitude versus Time measurement.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:TRIGger:LEVel:STATe { OFF ON 0 1 } DISPlay:AVTime:TRIGger:LEVel:STATe?
Arguments	OFF or 0 hides the power trigger level line. ON or 1 shows the power trigger level line.
Examples	DISPLAY:AVTIME:TRIGGER:LEVEL:STATE ON shows the power trigger level line on the screen.

DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe { OFF ON 0 1 } DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPLAY:AVTIME:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen in the Amplitude versus Time view.

DISPlay:AVTime:X:RSCale (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the Amplitude versus Time display.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:X:RSCale
Arguments	None
Examples	DISPLAY:AVTIME:X:RSCALE rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:AVTime:X[:SCALE]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the Amplitude versus Time view. Executing this command sets DISPlay:AVTime:X[:SCALE]:AUTO:STATe ON.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:X[:SCALE]:AUTO
Related Commands	DISPlay:AVTime:X[:SCALE]:AUTO:STATe
Arguments	None
Examples	DISPlay:AVTime:X:SCALE:AUTO sets the horizontal scale automatically to fit the waveform to the screen.

DISPlay:AVTime:X[:SCALE]:AUTO:STATe

Determines whether to set the horizontal scale automatically or manually.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:X[:SCALE]:AUTO:STATe { OFF ON 0 1 } DISPlay:AVTime:X[:SCALE]:AUTO:STATe?
Arguments	OFF or 0 specifies that the horizontal scale is set manually. To set it, use the DISPlay:AVTime:X[:SCALE]:FULL and DISPlay:AVTime:X[:SCALE]:OFFSet commands. ON or 1 specifies that the horizontal scale is set automatically.
Examples	DISPLAY:AVTIME:X:SCALE:AUTO:STATE ON specifies that the horizontal scale is set automatically.

DISPlay:AVTime:X[:SCALe]:FULL

Sets or queries the horizontal scale (full-scale time) of the Amplitude versus Time graph. Programming a specified scale sets DISPlay:AVTime:X[:SCALe] AUTO:STATe OFF.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:X[:SCALe]:FULL <value> DISPlay:AVTime:X[:SCALe]:FULL?
Related Commands	DISPlay:AVTime:X[:SCALe]:AUTO:STATe , DISPlay:AVTime:X[:SCALe]:OFFSet
Arguments	<value>::=<NRf> specifies the horizontal scale in full-scale time. Use the DISPlay:AVTime:X[:SCALe]:MAXimum? and DISPlay:AVTime:X[:SCALe]:MINimum? queries to get the upper and lower limits of the setting range.
Examples	DISPLAY:AVTIME:X:SCALE:FULL 25.6us sets the horizontal scale to 25.6 μ s.

DISPlay:AVTime:X[:SCALe]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:X[:SCALe]:MAXimum?
Related Commands	DISPlay:AVTime:X[:SCALe]:FULL
Arguments	None
Returns	<NRf> The upper limit of the horizontal scale setting range.

Examples `DISPLAY:AVTIME:X:SCALE:MAXIMUM?` might return `18.135E-3`, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

DISPlay:AVTime:X[:SCALe]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax `DISPlay:AVTime:X[:SCALe]:MINimum?`

Related Commands [DISPlay:AVTime:X\[:SCALe\]:FULL](#)

Arguments None

Returns <NRF> The lower limit of the horizontal scale setting range.

Examples `DISPLAY:AVTIME:X:SCALE:MINIMUM?` might return `10.0E-9`, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

DISPlay:AVTime:X[:SCALe]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the Amplitude versus Time graph. Programming a specified offset sets `DISPlay:AVTime:X[:SCALe] AUTO:STATe OFF`.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax `DISPlay:AVTime:X[:SCALe]:OFFSet <value>`
`DISPlay:AVTime:X[:SCALe]:OFFSet?`

Related Commands [DISPlay:AVTime:X\[:SCALe\]:AUTO:STATe](#), [DISPlay:AVTime:X\[:SCALe\]:FULL](#)

Arguments `<value>::=<Nrf>` specifies the minimum horizontal value. Use the [DISPlay:AVTime:X\[:SCALE\]:OFFSet:MAXimum?](#) and [DISPlay:AVTime:X\[:SCALE\]:OFFSet:MINimum?](#) queries to get the upper and lower limits of the setting range.

Examples `DISPlay:AVTIME:X:SCALE:OFFSET 800ns` sets the minimum horizontal value to 800 ns in the Amplitude versus Time graph.

DISPlay:AVTime:X[:SCALE]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax `DISPlay:AVTime:X[:SCALE]:OFFSet:MAXimum?`

Related Commands [DISPlay:AVTime:X\[:SCALE\]:OFFSet](#)

Arguments None

Returns `<Nrf>` The upper limit of the horizontal offset setting range.

Examples `DISPlay:AVTIME:X:SCALE:OFFSET:MAXIMUM?` might return `-1.812E-3`, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

DISPlay:AVTime:X[:SCALE]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax `DISPlay:AVTime:X[:SCALE]:OFFSet:MINimum?`

Related Commands [DISPlay:AVTime:X\[:SCALe\]:OFFSet](#)

Arguments None

Returns <NRF> The lower limit of the horizontal offset setting range.

Examples `DISPlay:AVTime:X:SCALE:OFFSET:MINIMUM?` might return `-16.28E-3`, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

DISPlay:AVTime:Y:RSCale (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Amplitude versus Time display.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax `DISPlay:AVTime:Y:RSCale`

Arguments None

Examples `DISPlay:AVTime:Y:RSCALE` rescales the vertical scale automatically to fit the waveform to the screen.

DISPlay:AVTime:Y[:SCALe]:FULL

Sets or queries the vertical range of the Amplitude versus Time graph.

Conditions Measurement views: Amplitude versus Time

Group Display commands

Syntax `DISPlay:AVTime:Y[:SCALe]:FULL <value>`
`DISPlay:AVTime:Y[:SCALe]:FULL?`

Related Commands	DISPlay:AVTime:Y[:SCALE]:OFFSet
Arguments	<value> ::= <NRf> specifies the vertical range. Range: 0.1 to 200 dB.
Examples	DISPLAY:AVTIME:Y:SCALE:FULL 100 sets the vertical range to 100 dB in the Amplitude versus Time graph.

DISPlay:AVTime:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the Amplitude versus Time graph.

Conditions	Measurement views: Amplitude versus Time
Group	Display commands
Syntax	DISPlay:AVTime:Y[:SCALE]:OFFSet <value> DISPlay:AVTime:Y[:SCALE]:OFFSet?

Related Commands	DISPlay:AVTime:Y[:SCALE]:FULL
Arguments	<value> ::= <NRf> specifies the vertical offset. Range: -170 to +50 dBm.
Examples	DISPLAY:AVTIME:Y:SCALE:OFFSET -12.5 sets the vertical offset to -12.5 dBm in the Amplitude versus Time graph.

DISPlay:CCDF:LEGend:STATe

Determines whether to show or hide the trace legend in the CCDF view. The legend indicates the trace detection and function on the screen for each displayed CCDF trace.

Conditions	Measurement views: CCDF
Group	Display commands

Syntax `DISPlay:CCDF:LEgEnd:StAte { OFF | ON | 0 | 1 }`
`DISPlay:CCDF:LEgEnd:StAte?`

Arguments OFF or 0 hides the trace legend.
 ON or 1 shows the trace legend.

Examples `DISPlay:CCDF:LEgEnd:StAte ON` shows the trace legend on the screen.

DISPlay:CCDF:WINDow:TRACe:GRATICule:GRID:StAte

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: CCDF

Group Display commands

Syntax `DISPlay:CCDF:WINDow:TRACe:GRATICule:GRID:StAte { OFF | ON`
`| 0 | 1 }`
`DISPlay:CCDF:WINDow:TRACe:GRATICule:GRID:StAte?`

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Examples `DISPlay:CCDF:WINDow:TRACe:GRATICule:GRID:StAte ON` shows the graticule grid on the screen in the CCDF view.

DISPlay:CONSt:MPHase

Sets or queries the multiplication constant of the phase multiplication constellation display for a CPM signal. This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to CPM.

Conditions Measurement views: Constellation

Group Display commands

Syntax `DISPlay:CONSte:MPHase { P1 | P2 | P4 | P8 | P16 | P32 }`
`DISPlay:CONSte:MPHase?`

Arguments The following table shows the arguments and phase multiplier.

Phase multiplication

Argument	Phase multiplier
P1	1
P2	2
P4	4
P8	8
P16	16
P32	32

Examples `DISPLAY:CONSTE:MPHASE P8` sets the phase multiplier to 8.

DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: Constellation

Group Display commands

Syntax `DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe { OFF | ON | 0 | 1 }`
`DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe?`

Arguments OFF or 0 hides the graticule grid.

ON or 1 shows the graticule grid.

Examples `DISPLAY:CONSTE:WINDOW:TRACE:GRATICULE:GRID:STATE ON` shows the graticule grid on the screen.

DISPlay:DDEMod:MEASview:DELeTe (No Query Form)

Deletes the measurement view in the general purpose digital modulation measurements.

Conditions Measurement views: General purpose digital modulation

Group Display commands

Syntax `DISPlay:DDEMod:MEASview:DELeTe { CONSte | DIQVtime | EDIagram | EVM | FDVTime | MERRor | PERRor | SIGNAqual | STABle | TDIagram }`

Arguments The following table lists the arguments. The arguments are the string type.

Table 2-30: Modulation measurement views

Argument	View
CONSte	Constellation
DIQVtime	Demodulated I&Q versus Time
EDIagram	Eye diagram
EVM	EVM (Error Vector Magnitude) versus Time
FDVTime	Frequency deviation versus Time
MERRor	Magnitude error versus Time
PERRor	Phase error versus Time
SIGNAqual	Signal quality
STABle	Symbol table
TDIagram	Trellis diagram

If you attempt to delete a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running" will be returned.

Examples `DISPlay:DDEMOD:MEASVIEW:DELETE CONSte` deletes the constellation view.

DISPlay:DDEMod:MEASview:NEW (No Query Form)

Displays a new measurement view in the general purpose digital modulation measurements.

Conditions Measurement views: General purpose digital modulation

Group Display commands

Syntax	<code>DISPlay:DDEMod:MEASview:NEW { CONSTe DIQVtime EDIagram EVM FDVTime MERRor PERRor SIGNALqual STABle TDIagram }</code>
Arguments	(See Table 2-30 on page 2-244.) If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.
Examples	<code>DISPLAY:DDEMOD:MEASVIEW:NEW CONSTe</code> creates the constellation view.

DISPlay:DDEMod:MEASview:SElect

Selects a measurement view in the general purpose digital modulation measurements on the screen. The query command returns the currently selected view.

Selecting a measurement optimizes it. Other measurements may be optimized as a side effect. Refer to the [DISPlay:WINDow:OPTimized:MEASurement?](#) query.

Conditions	Measurement views: General purpose digital modulation
Group	Display commands
Syntax	<code>DISPlay:DDEMod:MEASview:SElect { CONSTe DIQVtime EDIagram EVM FDVTime MERRor PERRor SIGNALqual STABle TDIagram }</code> <code>DISPlay:DDEMod:MEASview:SElect?</code>
Arguments	(See Table 2-30 on page 2-244.) If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.
Examples	<code>DISPLAY:DDEMOD:MEASVIEW:SELECT CONSTe</code> selects the constellation view.

DISPlay:DDEMod:RADix

Sets or queries the base of symbols. This command is effective in the symbol table.

Conditions	Measurement views: Symbol table
-------------------	---------------------------------

Group	Display commands
Syntax	DISP <code>l</code> ay:DDEMod:RADiX { BINary HEXadecima <code>l</code> } DISP <code>l</code> ay:DDEMod:RADiX?
Arguments	BINary selects binary notation. HEXadecima <code>l</code> selects hexadecimal notation.
Examples	DISP <code>l</code> AY:DDEMOD:RADIX BINary selects binary notation for the symbol table.

DISP`l`ay:DDEMod:X[:SCALe]

Sets or queries the horizontal scale (full-scale time) for the time measurements in the general purpose digital modulation analysis. Programming a specified scale sets DISP`l`ay:DDEMod:X[:SCALe]:AUTO:STATe OFF.

Conditions	Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:DDEMod:X[:SCALe] <va <code>l</code> ue> DISP <code>l</code> ay:DDEMod:X[:SCALe]?
Related Commands	DISP<code>l</code>ay:DDEMod:X[:SCALe]:AUTO:STATe , DISP<code>l</code>ay:DDEMod:X[:SCALe]:OFFSet
Arguments	<va <code>l</code> ue>::=<NRf> specifies the horizontal scale in full-scale time. Use the DISP<code>l</code>ay:DDEMod:X[:SCALe]:MAXimum? and DISP<code>l</code>ay:DDEMod:X[:SCALe]:MINimum? queries to get the upper and lower limits of the setting range. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	DISP <code>l</code> AY:DDEMOD:X:SCALE 1.5us sets the horizontal scale to 1.5 μ s.

DISPlay:DDEMod:X[:SCALE]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the general purpose digital modulation analysis. Executing this command sets DISPlay:DDEMod:X[:SCALE]:AUTO:STATE ON.

Conditions Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time

Group Display commands

Syntax DISPlay:DDEMod:X[:SCALE]:AUTO

Related Commands [DISPlay:DDEMod:X\[:SCALE\]:AUTO:STATE](#)

Arguments None

Examples DISPLAY:DDEMOD:X:SCALE:AUTO sets the horizontal scale automatically to fit the waveform to the screen.

DISPlay:DDEMod:X[:SCALE]:AUTO:STATE

Determines whether to set the horizontal scale automatically or manually.

Conditions Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time

Group Display commands

Syntax DISPlay:DDEMod:X[:SCALE]:AUTO:STATE { OFF | ON | 0 | 1 }
DISPlay:DDEMod:X[:SCALE]:AUTO:STATE?

Arguments OFF or 0 specifies that the horizontal scale is set manually. To set it, use the [DISPlay:DDEMod:X\[:SCALE\]](#) and [DISPlay:DDEMod:X\[:SCALE\]:OFFSet](#) commands.

ON or 1 specifies that the horizontal scale is set automatically.

Examples `DISPLAY:DDEMOD:X:SCALE:AUTO:STATE ON` specifies that the horizontal scale is set automatically.

DISPlay:DDEMod:X[:SCALe]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Conditions Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time

Group Display commands

Syntax `DISPlay:DDEMod:X[:SCALe]:MAXimum?`

Arguments None

Returns <NRF> The upper limit of the horizontal scale setting range.
The unit can be changed by the [\[SENSe\]:DDEMod:TIME:UNITs](#) command.

Examples `DISPLAY:DDEMOD:X:SCALE:MAXIMUM?` might return `18.135E-3`, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

DISPlay:DDEMod:X[:SCALe]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Conditions Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time

Group Display commands

Syntax `DISPlay:DDEMod:X[:SCALe]:MINimum?`

Arguments None

Returns <NRF> The lower limit of the horizontal scale setting range.
The unit can be changed by the [\[SENSe\]:DDEMod:TIME:UNITs](#) command.

Examples `DISPLAY:DDEMOD:X:SCALE:MINIMUM` might return `10.0E-9`, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

DISPlay:DDEMod:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) for the time measurements in the general purpose digital modulation analysis. Programming a specified offset sets `DISPlay:DDEMod:X[:SCALE]:AUTO:STATe` OFF.

Conditions Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time

Group Display commands

Syntax `DISPlay:DDEMod:X[:SCALE]:OFFSet <value>`
`DISPlay:DDEMod:X[:SCALE]:OFFSet?`

Related Commands [DISPlay:DDEMod:X\[:SCALE\]:AUTO:STATe](#), [DISPlay:DDEMod:X\[:SCALE\]](#)

Arguments `<value>::=<Nrf>` specifies the minimum horizontal value.

Use the [DISPlay:DDEMod:X\[:SCALE\]:OFFSet:MAXimum?](#) and [DISPlay:DDEMod:X\[:SCALE\]:OFFSet:MINimum?](#) queries to get the upper and lower limits of the setting range.

The unit can be changed by the [\[SENSe\]:DDEMod:TIME:UNITs](#) command.

Examples `DISPLAY:DDEMOD:X:SCALE:OFFSET 20.075us` sets the minimum horizontal value to 20.075 μ s.

DISPlay:DDEMod:X[:SCALE]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Conditions Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time

Group Display commands

Syntax `DISPlay:DDEMod:X[:SCALE]:OFFSet:MAXimum?`

Arguments	None
Returns	<NRF> The upper limit of the horizontal offset setting range. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	DISPLAY:DDEMOD:X:SCALE:OFFSET:MAXIMUM? might return -1.812E-3, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

DISPlay:DDEMod:X[:SCALE]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Conditions	Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:DDEMod:X[:SCALE]:OFFSet:MINimum?
Arguments	None
Returns	<NRF> The lower limit of the horizontal offset setting range. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	DISPLAY:DDEMOD:X:SCALE:OFFSET:MINIMUM? might return -16.28E-3, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

DISPlay:DDEMod:X[:SCALE]:RESet (No Query Form)

Presets the horizontal scale to the default value for the time measurements in the general purpose digital modulation analysis.

Conditions	Measurement views: EVM versus Time, Magnitude error versus Time, Phase error versus Time
Group	Display commands

Syntax	DISP <code>l</code> ay:DDEMod:X[:SCALE]:RESet
Arguments	None
Examples	DISP <code>l</code> ay:DDEMOD:X:SCALE:RESEt presets the horizontal scale to the default value.

DISP`l`ay:DIAGram:X[:SCALE]

Sets or queries the horizontal range for the eye and trellis diagrams in the general purpose digital modulation analysis.

Conditions	Measurement views: Eye diagram, Trellis diagram
Group	Display commands
Syntax	DISP <code>l</code> ay:DIAGram:X[:SCALE] <value> DISP <code>l</code> ay:DIAGram:X[:SCALE]?
Arguments	<value> ::= <NR1> specifies the horizontal range. Range: 1 to 16 symbols.
Examples	DISP <code>l</code> ay:DIAGRAM:X:SCALE 3 sets the horizontal range to 3 symbols in the eye and trellis diagrams.

DISP`l`ay:DIAGram:X[:SCALE]:RESet (No Query Form)

Presets the horizontal scale to the default value for the eye and trellis diagrams in the general purpose digital modulation analysis.

Conditions	Measurement views: Eye diagram, Trellis diagram
Group	Display commands
Syntax	DISP <code>l</code> ay:DIAGram:X[:SCALE]:RESet
Arguments	None

Examples `DISPLAY:DIAGRAM:X:SCALE:RESET` presets the horizontal scale to the default value for the eye and trellis diagrams.

DISPlay:DIQVtime:WINDow:TRACe:GRATICule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: Demodulated I&Q versus Time

Group Display commands

Syntax `DISPlay:DIQVtime:WINDow:TRACe:GRATICule:GRID:STATE { OFF | ON | 0 | 1 }`
`DISPlay:DIQVtime:WINDow:TRACe:GRATICule:GRID:STATE?`

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Examples `DISPLAY:DIQVTIME:WINDOW:TRACE:GRATICULE:GRID:STATE ON` shows the graticule grid on the screen in the Demodulated I&Q versus Time view.

DISPlay:DIQVtime:Y[:SCALE]

Sets or queries the vertical range of the Demodulated I&Q versus Time graph.

Conditions Measurement views: Demodulated I&Q versus Time

Group Display commands

Syntax `DISPlay:DIQVtime:Y[:SCALE] <value>`
`DISPlay:DIQVtime:Y[:SCALE]?`

Arguments `<value>::=<NRF>` specifies the vertical range. Range: 1 μ V to 10 V.

Examples `DISPLAY:DIQVTIME:Y:SCALE 2.5` sets the vertical range to 2.5 V in the Demodulated I&Q versus Time graph.

DISPlay:DIQVtime:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Demodulated I&Q versus Time display.

Conditions	Measurement views: Demodulated I&Q versus Time
Group	Display commands
Syntax	DISPlay:DIQVtime:Y[:SCALe]:AUTO
Arguments	None
Examples	DISPLAY:DIQVTIME:Y:SCALE:AUTO sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:DIQVtime:Y[:SCALe]:OFFSet

Sets or queries the vertical offset (center point of the vertical axis) of the Demodulated I&Q versus Time graph.

Conditions	Measurement views: Demodulated I&Q versus Time
Group	Display commands
Syntax	DISPlay:DIQVtime:Y[:SCALe]:OFFSet <value> DISPlay:DIQVtime:Y[:SCALe]:OFFSet?
Arguments	<value> ::= <NRF> specifies the vertical offset. Range: -5 to +5 V.
Examples	DISPLAY:DIQVTIME:Y:SCALE:OFFSET -0.5 sets the vertical offset to -0.5 V in the Demodulated I&Q versus Time graph.

DISPlay:DPSA:LEGend:STATe

Determines whether to show or hide the trace legend on the display. The legend indicates the trace detection and function on the screen for each displayed trace.

Conditions	Measurement views: DPX spectrum
Group	Display commands
Syntax	DISPlay:DPSA:LEGend:STATE { OFF ON 0 1 } DISPlay:DPSA:LEGend:STATE?
Arguments	OFF or 0 hides the trace legend. ON or 1 shows the trace legend.
Examples	DISPLAY:DPSA:LEGEND:STATE ON shows the trace legend on the screen.

DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: DPX spectrum
Group	Display commands
Syntax	DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATE { OFF ON 0 1 } DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPLAY:DPSA:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen in the DPX spectrum view.

DISPlay:DPSA:Y[:SCALe]:PDIVision

Sets or queries the vertical scale (per division) in the DPX spectrum view.

Conditions	Measurement views: DPX spectrum
-------------------	---------------------------------

Group	Display commands
Syntax	DISP <code>lay:DPSA:Y[:SCALE]:PDIVision</code> <value> DISP <code>lay:DPSA:Y[:SCALE]:PDIVision?</code>
Related Commands	[SENSe]:POWer:UNITs
Arguments	<value> ::= <NRf> specifies the vertical scale (per division). Range: 2 to 20 dB/div.
Examples	SENSE:DPSA:Y:SCALE:PDIVISION 0.5 sets the vertical scale to 0.5 dB/div.

DISP`lay:EDIagram:WINDow:TRACe:GRATICule:GRID:STATE`

Determines whether to show or hide the graticule grid on the screen in the eye diagram.

Conditions	Measurement views: Eye diagram
Group	Display commands
Syntax	DISP <code>lay:EDIagram:WINDow:TRACe:GRATICule:GRID:STATE</code> { OFF ON 0 1 } DISP <code>lay:EDIagram:WINDow:TRACe:GRATICule:GRID:STATE?</code>
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPLAY:EDIAGRAM:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen in the eye diagram.

DISP`lay:EDIagram:Y[:SCALE]`

Sets or queries the vertical range of the eye diagram.

Conditions	Measurement views: Eye diagram
-------------------	--------------------------------

Group	Display commands
Syntax	DISP <code>lay</code> :EDIagram:Y[:SCALE] <value> DISP <code>lay</code> :EDIagram:Y[:SCALE]?
Arguments	<value>::=<NRF> specifies the vertical range. Range: 1 μ to 100 (unitless).
Examples	DISP <code>lay</code> :EDIAGRAM:Y:SCALE 2.5 sets the vertical range to 2.5 in the eye diagram.

DISP`lay`:EDiagram:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the eye diagram.

Conditions	Measurement views: Eye diagram
Group	Display commands
Syntax	DISP <code>lay</code> :EDIagram:Y[:SCALE]:AUTO
Arguments	None
Examples	DISP <code>lay</code> :EDIAGRAM:Y:SCALE:AUTO sets the vertical scale automatically to fit the waveform to the screen.

DISP`lay`:EDiagram:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (center point of the vertical axis) of the eye diagram.

Conditions	Measurement views: Eye diagram
Group	Display commands
Syntax	DISP <code>lay</code> :EDIagram:Y[:SCALE]:OFFSet <value> DISP <code>lay</code> :EDIagram:Y[:SCALE]:OFFSet?

Arguments <value> ::= <Nrf> specifies the minimum vertical value.
Range: -50 to +50 (unitless).

Examples DISPLAY:EDIAGRAM:Y:SCALE:OFFSET -0.5 sets the vertical offset to -0.5 in the eye diagram.

DISPlay:EVM:WINDow:TRACe:GRATICule:GRID:STATE

Sets or queries the graticule grid view state for the EVM view.

Conditions Measurement views: EVM versus Time

Group Display commands

Syntax DISPlay:EVM:WINDow:TRACe:GRATICule:GRID:STATE { OFF | ON |
0 | 1 }
DISPlay:EVM:WINDow:TRACe:GRATICule:GRID:STATE?

Arguments OFF or 0 hides the graticule grid.
ON or 1 shows the graticule grid.

Examples DISPLAY:EVM:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the EVM view.

DISPlay:EVM:Y[:SCALE]

Sets or queries the vertical range of the EVM versus Time graph.

Conditions Measurement views: EVM versus Time

Group Display commands

Syntax DISPlay:EVM:Y[:SCALE] <value>
DISPlay:EVM:Y[:SCALE]?

Related Commands [DISPlay:EVM:Y\[:SCALE\]:OFFSet](#)

Arguments <value>::=<Nrf> specifies the vertical range. Range: 1 to 100%.

Examples DISPLAY:EVM:Y:SCALE 50 sets the vertical range to 50% in the EVM versus Time graph.

DISPlay:EVM:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the EVM versus Time display.

Conditions Measurement views: EVM versus Time

Group Display commands

Syntax DISPlay:EVM:Y[:SCALE]:AUTO

Arguments None

Examples DISPLAY:EVM:Y:SCALE:AUTO sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:EVM:Y[:SCALE]:OFFSet

Sets or queries the minimum vertical value (bottom edge) of the EVM versus Time graph.

Conditions Measurement views: EVM versus Time

Group Display commands

Syntax DISPlay:EVM:Y[:SCALE]:OFFSet <value>
DISPlay:EVM:Y[:SCALE]:OFFSet?

Related Commands [DISPlay:EVM:Y\[:SCALE\]](#)

Arguments <value>::=<Nrf> specifies the minimum vertical value. Range: -100 to 100%.

Examples `DISPLAY:EVM:Y:SCALE:OFFSET -9.5` sets the minimum vertical value to -9.5% in the EVM versus Time graph.

DISPlay:FDVTime:WINDow:TRACe:GRATICule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: Frequency deviation versus Time

Group Display commands

Syntax `DISPlay:FDVTime:WINDow:TRACe:GRATICule:GRID:STATe { OFF | ON | 0 | 1 }`
`DISPlay:FDVTime:WINDow:TRACe:GRATICule:GRID:STATe?`

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Examples `DISPLAY:FDVTIME:WINDOW:TRACE:GRATICULE:GRID:STATE ON` shows the graticule grid on the Frequency deviation versus Time view.

DISPlay:FDVTime:Y[:SCALE]

Sets or queries the vertical range of the Frequency deviation versus Time graph.

Conditions Measurement views: Frequency deviation versus Time

Group Display commands

Syntax `DISPlay:FDVTime:Y[:SCALE] <value>`
`DISPlay:FDVTime:Y[:SCALE]?`

Arguments `<value> ::= <Nrf>` specifies the vertical range. Range: 10 Hz to 120 MHz.

Examples `DISPLAY:FDVTIME:Y:SCALE 30MHZ` sets the vertical range to 30 MHz in the Frequency deviation versus Time graph.

DISPlay:FDVTime:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Frequency deviation versus Time view.

Conditions	Measurement views: Frequency deviation versus Time
Group	Display commands
Syntax	DISPlay:FDVTime:Y[:SCALE]:AUTO
Arguments	None
Examples	DISPLAY:FDVTIME:Y:SCALE:AUTO sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:FDVTime:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (center point of the vertical axis) in the Frequency deviation versus Time graph.

Conditions	Measurement views: Frequency deviation versus Time
Group	Display commands
Syntax	DISPlay:FDVTime:Y[:SCALE]:OFFSet <value> DISPlay:FDVTime:Y[:SCALE]:OFFSet?
Arguments	<value>::=<NRF> specifies the vertical offset. Range: -60 MHz to +60 MHz.
Examples	DISPLAY:FDVTIME:Y:SCALE:OFFSET -14.5MHZ sets the vertical offset to -14.5 MHz in the Frequency deviation versus Time graph.

DISPlay:FVTime:WINDow:TRACe:GRATICule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Frequency versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:FVTime:WINDow:TRACe:GRATICule:GRID:STATE { OFF ON 0 1 } DISP <code>l</code> ay:FVTime:WINDow:TRACe:GRATICule:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISP <code>l</code> AY:FVTIME:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the Frequency versus Time view.

DISP`l`ay:FVTime:X[:SCALE]

Sets or queries the horizontal scale (full-scale time) of the Frequency versus Time graph. Programming a specified scale sets DISP`l`ay:FVTime:X[:SCALE] AUTO:STATe OFF.

Conditions	Measurement views: Frequency versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:FVTime:X[:SCALE] <value> DISP <code>l</code> ay:FVTime:X[:SCALE]?
Related Commands	DISP <code>l</code> ay:FVTime:X[:SCALE]:AUTO:STATe, DISP <code>l</code> ay:FVTime:X[:SCALE]:OFFSet
Arguments	<value>::={ <NRF> MAXimum MINimum } specifies the horizontal scale in full-scale time. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively. Use the DISP <code>l</code> ay:FVTime:X[:SCALE]:MAXimum? and DISP <code>l</code> ay:FVTime:X[:SCALE]:MINimum? queries to get the upper and lower limit values of the setting range.
Examples	DISP <code>l</code> AY:FVTIME:X:SCALE 25.6us sets the horizontal scale to 25.6 μ s.

DISPlay:FVTime:X[:SCALe]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the Frequency versus Time view. Executing this command sets DISPlay:FVTime X[:SCALe]:AUTO:STATe ON.

Conditions	Measurement views: Frequency versus Time
Group	Display commands
Syntax	DISPlay:FVTime:X[:SCALe]:AUTO
Related Commands	DISPlay:FVTime:X[:SCALe]:AUTO:STATe
Arguments	None
Examples	DISPLAY:FVTIME:X:SCALE:AUTO sets the horizontal scale automatically to fit the waveform to the screen.

DISPlay:FVTime:X[:SCALe]:AUTO:STATe

Determines whether to set the horizontal scale automatically or manually.

Conditions	Measurement views: Frequency versus Time
Group	Display commands
Syntax	DISPlay:FVTime:X[:SCALe]:AUTO:STATe { OFF ON 0 1 } DISPlay:FVTime:X[:SCALe]:AUTO:STATe?
Arguments	OFF or 0 specifies that the horizontal scale is set manually. To set it, use the DISPlay:FVTime:X[:SCALe] and DISPlay:FVTime:X[:SCALe]:OFFSet commands. ON or 1 specifies that the horizontal scale is set automatically.
Examples	DISPLAY:FVTIME:X:SCALE:AUTO:STATE ON specifies that the horizontal scale is set automatically.

DISPlay:FVTime:X[:SCALe]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Conditions Measurement views: Frequency versus Time

Group Display commands

Syntax DISPlay:FVTime:X[:SCALe]:MAXimum?

Related Commands [DISPlay:FVTime:X\[:SCALe\]](#)

Arguments None

Returns <NRf> The upper limit of the horizontal scale setting range.

Examples DISPLAY:FVTIME:X:SCALE:MAXIMUM? might return 18.135E-3, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

DISPlay:FVTime:X[:SCALe]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Conditions Measurement views: Frequency versus Time

Group Display commands

Syntax DISPlay:FVTime:X[:SCALe]:MINimum?

Related Commands [DISPlay:FVTime:X\[:SCALe\]](#)

Arguments None

Returns <NRf> The lower limit of the horizontal scale setting range.

Examples `DISPLAY:FVTIME:X:SCALE:MINIMUM?` might return `10.0E-9`, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

`DISPlay:FVTime:X[:SCALe]:OFFSet`

Sets or queries the minimum horizontal value (left edge) of the Frequency versus Time graph. Programming a specified offset sets `DISPlay:FVTime:X[:SCALe] AUTO:STATe OFF`.

Conditions Measurement views: Frequency versus Time

Group Display commands

Syntax `DISPlay:FVTime:X[:SCALe]:OFFSet <value>`
`DISPlay:FVTime:X[:SCALe]:OFFSet?`

Related Commands [DISPlay:FVTime:X\[:SCALe\]:AUTO:STATe](#), [DISPlay:FVTime:X\[:SCALe\]](#)

Arguments `<value>::={ <Nrf> | MAXimum | MINimum }` specifies the horizontal offset. `MAXimum` and `MINimum` represent the upper and lower limits of the setting range, respectively.

Use the [DISPlay:FVTime:X\[:SCALe\]:OFFSet:MAXimum?](#) and [DISPlay:FVTime:X\[:SCALe\]:OFFSet:MINimum?](#) queries to get the upper and lower limit values of the setting range.

Examples `DISPLAY:FVTIME:X:SCALE:OFFSET 800ns` sets the minimum horizontal value to 800 ns in the Frequency versus Time graph.

`DISPlay:FVTime:X[:SCALe]:OFFSet:MAXimum? (Query Only)`

Queries the upper limit of the horizontal offset setting range.

Conditions Measurement views: Frequency versus Time

Group Display commands

Syntax `DISPlay:FVTime:X[:SCALe]:OFFSet:MAXimum?`

Related Commands	DISPlay:FVTime:X[:SCALE]:OFFSet
Arguments	None
Returns	<NRf> The upper limit of the horizontal offset setting range.
Examples	DISPLAY:FVTIME:X:SCALE:OFFSET:MAXIMUM? might return -1.812E-3, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

DISPlay:FVTime:X[:SCALE]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Conditions	Measurement views: Frequency versus Time
Group	Display commands
Syntax	DISPlay:FVTime:X[:SCALE]:OFFSet:MINimum?
Related Commands	DISPlay:FVTime:X[:SCALE]:OFFSet
Arguments	None
Returns	<NRf> The lower limit of the horizontal offset setting range.
Examples	DISPLAY:FVTIME:X:SCALE:OFFSET:MINIMUM? might return -16.28E-3, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

DISPlay:FVTime:Y[:SCALE]

Sets or queries the vertical range of the Frequency versus Time graph.

Conditions	Measurement views: Frequency versus Time
Group	Display commands

Syntax `DISPlay:FVTime:Y[:SCALE] <value>`
`DISPlay:FVTime:Y[:SCALE]?`

Related Commands [DISPlay:FVTime:Y\[:SCALE\]:OFFSet](#)

Arguments `<value>::=<NRF>` specifies the vertical range. Range: 10 Hz to 120 MHz.

Examples `DISPlay:FVTime:Y:SCALE 30MHZ` sets the vertical range to 30 MHz in the Frequency versus Time graph.

DISPlay:FVTime:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Frequency versus Time view.

Conditions Measurement views: Frequency versus Time

Group Display commands

Syntax `DISPlay:FVTime:Y[:SCALE]:AUTO`

Arguments None

Examples `DISPlay:FVTime:Y:SCALE:AUTO` sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:FVTime:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the center of the vertical axis) in the Frequency versus Time graph.

Conditions Measurement views: Frequency versus Time

Group Display commands

Syntax `DISPlay:FVTime:Y[:SCALE]:OFFSet <value>`
`DISPlay:FVTime:Y[:SCALE]:OFFSet?`

Related Commands [DISPlay:FVTime:Y\[:SCALE\]](#)

Arguments `<value>::=<NRF>` specifies the vertical offset. Range: -60 MHz to +60 MHz.

Examples `DISPlay:FVTime:Y:SCALE:OFFSET -14.5MHz` sets the vertical offset to -14.5 MHz in the Frequency versus Time graph.

DISPlay:GENeral:MEASview:DElete (No Query Form)

Deletes a measurement view in the general signal viewing.

Conditions Measurement views: General signal viewing

Group Display commands

Syntax `DISPlay:GENeral:MEASview:DElete { SPECTrum | DPsa | AVTime | FVTime | PHVTime | IQVTime | SGRam | TOVerview }`

Arguments The following table shows the arguments. The arguments are the string type.

Table 2-31: General signal viewing views

Argument	View
SPECTrum	Spectrum
DPsa	DPX (Digital Phosphor) spectrum
AVTime	Amplitude versus Time
FVTime	Frequency versus Time
PHVTime	Phase versus Time
IQVTime	IQ versus Time
SGRam	Spectrogram
TOVerview	Time overview

If you attempt to delete a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Examples `DISPlay:GENeral:MEASVIEW:DELETE DPsa` deletes the DPX spectrum view.

DISPlay:GENeral:MEASview:NEW (No Query Form)

Displays a new measurement view in the general signal viewing.

Conditions	Measurement views: General signal viewing
Group	Display commands
Syntax	DISPlay:GENeral:MEASview:NEW { SPECTrum DPSA AVTime FVTime PHVTime IQVTime SGRam TOVerview }
Arguments	(See Table 2-31 on page 2-267.) If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.
Examples	DISPLAY:GENERAL:MEASVIEW:NEW DPSA creates the DPX spectrum view.

DISPlay:GENeral:MEASview:SELEct

Selects a measurement view in the general signal viewing on the screen. The query command returns the currently selected view.

Selecting a measurement optimizes it. Other measurements may be optimized as a side effect. Refer to the [DISPlay:WINDow:OPTimized:MEASurement?](#) query.

Conditions	Measurement views: General signal viewing
Group	Display commands
Syntax	DISPlay:GENeral:MEASview:SELEct { SPECTrum DPSA AVTime FVTime PHVTime IQVTime SGRam TOVerview } DISPlay:GENeral:MEASview:SELEct?
Arguments	(See Table 2-31 on page 2-267.) If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned. The time overview (TOVerview) cannot be selected as the primary measurement. If you select it, the error (-200, "Execution error; Time Overview cannot be Primary measurement") will be returned. If you use the DISPlay:GENeral MEASview:SELEct? query with the time overview as the only measurement

active, the error (-200, "Execution error; Analysis selected is not running") will be returned.

Examples `DISPLAY:GENERAL:MEASVIEW:SELECT DPXA` selects the DPX spectrum view.

DISPlay:GPRF:MEASview:DELeTe (No Query Form)

Deletes a selected measurement view in the RF measurements.

Conditions Measurement views: RF measurements

Group Display commands

Syntax `DISPlay:GPRF:MEASview:DELeTe { CCDF | ACPower | MCPower | OBW | PNOise | SPURious }`

Arguments `CCDF` deletes the CCDF view.

`ACPower` deletes the Channel power and ACPR view.

`MCPower` deletes the MCPR view.

`OBW` deletes the Occupied Bandwidth view.

`PNOise` deletes the Phase Noise view (Option 11 only).

`SPURious` deletes the Spurious view.

If you attempt to delete a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Examples `DISPLAY:GPRF:MEASVIEW:DELETE ACPower` deletes the Channel power and ACPR view.

DISPlay:GPRF:MEASview:NEw (No Query Form)

Displays a new measurement view in the RF measurements.

Conditions Measurement views: RF measurements

Group Display commands

Syntax `DISPlay:GPRF:MEASview:NEW { CCDF | ACPower | MCPower | OBW | PNOise | SPURious }`

Arguments CCDF opens the CCDF view.
 ACPower opens the Channel power and ACPR view.
 MCPower opens the MCPR view.
 OBW opens the Occupied Bandwidth view.
 PNOise opens the Phase Noise view (Option 11 only).
 SPURious opens the Spurious view.
 If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.

Examples `DISPLAY:GPRF:MEASVIEW:NEW ACPower` creates the Channel power and ACPR view.

DISPlay:GPRF:MEASview:SElect

Selects a measurement view in the RF measurements on the screen. The query command returns the currently selected view.

Selecting a measurement optimizes it. Other measurements may be optimized as a side effect. Refer to the [DISPlay:WINDow:OPTimized:MEASurement?](#) query.

Conditions Measurement views: RF measurements

Group Display commands

Syntax `DISPlay:GPRF:MEASview:SElect { CCDF | ACPower | MCPower | OBW | PNOise | SPURious }`
`DISPlay:GPRF:MEASview:SElect?`

Arguments CCDF selects the CCDF view.
 ACPower selects the Channel power and ACPR view.
 MCPower selects the MCPR view.
 OBW selects the Occupied Bandwidth view.
 PNOise selects the Phase Noise view (Option 11 only).

SPURious selects the Spurious view.

If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Examples `DISPlay:GPRF:MEASVIEW:SELECT ACPower` selects the Channel power and ACPR view.

DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATE

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax `DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATE { OFF | ON | 0 | 1 }`
`DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATE?`

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Examples `DISPlay:IQVTIME:WINDOW:TRACE:GRATICULE:GRID:STATE ON` shows the graticule grid on the RF I&Q versus Time view.

DISPlay:IQVTime:X[:SCALE]

Sets or queries the horizontal scale (full-scale time) of the RF I&Q versus Time graph. Programming a specified scale sets `DISPlay:IQVTime:X[:SCALE] AUTO:STATE OFF`.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax `DISPlay:IQVTime:X[:SCALE] <value>`
`DISPlay:IQVTime:X[:SCALE]?`

Related Commands [DISPlay:IQVTime:X\[:SCALE\]:AUTO:STATe](#), [DISPlay:IQVTime:X\[:SCALE\]:OFFSet](#)

Arguments `<value>::={ <NRF> | MAXimum | MINimum }` specifies the horizontal scale in full-scale time. `MAXimum` and `MINimum` represent the upper and lower limits of the setting range, respectively. Use the [DISPlay:IQVTime:X\[:SCALE\]:MAXimum?](#) and [DISPlay:IQVTime:X\[:SCALE\]:MINimum?](#) queries to get the upper and lower limit values of the setting range.

Examples `DISPLAY:IQVTIME:X:SCALE 100us` sets the horizontal scale to 100 μ s.

DISPlay:IQVTime:X[:SCALE]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the RF I&Q versus Time view. Executing this command sets `DISPlay:IQVTime X[:SCALE]:AUTO:STATe ON`.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax `DISPlay:IQVTime:X[:SCALE]:AUTO`

Related Commands [DISPlay:IQVTime:X\[:SCALE\]](#), [DISPlay:IQVTime:X\[:SCALE\]:AUTO:STATe](#)

Arguments None

Examples `DISPLAY:IQVTIME:X:SCALE:AUTO` sets the horizontal scale automatically to fit the waveform to the screen.

DISPlay:IQVTime:X[:SCALE]:AUTO:STATe

Determines whether to set the horizontal scale automatically or manually.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax	<code>DISPlay:IQVTime:X[:SCALE]:AUTO:STATE { OFF ON 0 1 }</code> <code>DISPlay:IQVTime:X[:SCALE]:AUTO:STATE?</code>
Arguments	OFF or 0 specifies that the horizontal scale is set manually. To set it, use the DISPlay:IQVTime:X[:SCALE] and DISPlay:IQVTime:X[:SCALE]:OFFSet commands. ON or 1 specifies that the horizontal scale is set automatically.
Examples	<code>DISPLAY:IQVTIME:X:SCALE:AUTO:STATE ON</code> specifies that the horizontal scale is set automatically.

DISPlay:IQVTime:X[:SCALE]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Conditions	Measurement views: RF I&Q versus Time
Group	Display commands
Syntax	<code>DISPlay:IQVTime:X[:SCALE]:MAXimum?</code>
Related Commands	DISPlay:IQVTime:X[:SCALE]
Arguments	None
Returns	<Nrf> The upper limit of the horizontal scale setting range.
Examples	<code>DISPLAY:IQVTIME:X:SCALE:MAXIMUM?</code> might return <code>18.135E-3</code> , indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

DISPlay:IQVTime:X[:SCALE]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Conditions	Measurement views: RF I&Q versus Time
Group	Display commands

Syntax `DISPlay:IQVTime:X[:SCALE]:MINimum?`

Related Commands [DISPlay:IQVTime:X\[:SCALE\]](#)

Arguments None

Returns <NRF> The lower limit of the horizontal scale setting range.

Examples `DISPLAY:IQVTIME:X:SCALE:MINIMUM?` might return `10.0E-9`, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

DISPlay:IQVTime:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the RF I&Q versus Time graph. Programming a specified offset sets `DISPlay:IQVTime:X[:SCALE] AUTO:STATe OFF`.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax `DISPlay:IQVTime:X[:SCALE]:OFFSet <value>`
`DISPlay:IQVTime:X[:SCALE]:OFFSet?`

Related Commands [DISPlay:IQVTime:X\[:SCALE\]:AUTO:STATe](#), [DISPlay:IQVTime:X\[:SCALE\]](#)

Arguments `<value>::={ <NRF> | MAXimum | MINimum }` specifies the horizontal offset. `MAXimum` and `MINimum` represent the upper and lower limits of the setting range, respectively.

Use the [DISPlay:IQVTime:X\[:SCALE\]:OFFSet:MAXimum?](#) and [DISPlay:IQVTime:X\[:SCALE\]:OFFSet:MINimum?](#) queries to get the upper and lower limit values of the setting range.

Examples `DISPLAY:IQVTIME:X:SCALE:OFFSET 800ns` sets the minimum horizontal value to 800 ns in the RF I&Q versus Time graph.

DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum?

Related Commands [DISPlay:IQVTime:X\[:SCALe\]:OFFSet](#)

Arguments None

Returns <NRf> The upper limit of the horizontal offset setting range.

Examples DISPlay:IQVTime:X:SCALE:OFFSet:MAXimum? might return -1.812E-3, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

DISPlay:IQVTime:X[:SCALe]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax DISPlay:IQVTime:X[:SCALe]:OFFSet:MINimum?

Related Commands [DISPlay:IQVTime:X\[:SCALe\]:OFFSet](#)

Arguments None

Returns <NRf> The lower limit of the horizontal offset setting range.

Examples `DISPLAY:IQVTIME:X:SCALE:OFFSET:MINIMUM?` might return `-16.28E-3`, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

DISPlay:IQVTime:Y[:SCALE]

Sets or queries the vertical range of the RF I&Q versus Time graph.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax `DISPlay:IQVTime:Y[:SCALE] <value>`
`DISPlay:IQVTime:Y[:SCALE]?`

Related Commands [DISPlay:IQVTime:Y\[:SCALE\]:OFFSet](#)

Arguments `<value>::=<Nrf>` specifies the vertical range. Range: 1 μ to 10 V.

Examples `DISPLAY:IQVTIME:Y:SCALE 1.5` sets the vertical range to 1.5 V in the RF I&Q versus Time graph.

DISPlay:IQVTime:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the RF I&Q versus Time view.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax `DISPlay:IQVTime:Y[:SCALE]:AUTO`

Arguments None

Examples `DISPLAY:IQVTIME:Y:SCALE:AUTO` sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:IQVTime:Y[:SCALe]:OFFSet

Sets or queries the vertical offset (the value at the center of the vertical axis) in the RF I&Q versus Time graph.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax DISPlay:IQVTime:Y[:SCALe]:OFFSet <value>
DISPlay:IQVTime:Y[:SCALe]:OFFSet?

Related Commands [DISPlay:IQVTime:Y\[:SCALe\]](#)

Arguments <value>::=<Nrf> specifies the vertical offset. Range: -5 to +5 V.

Examples DISPLAY:IQVTIME:Y:SCALE:OFFSET -82.75mV sets the vertical offset to -82.75 mV in the RF I&Q versus Time graph.

DISPlay:IQVTime:Y[:SCALe]:RESCale (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen.

Conditions Measurement views: RF I&Q versus Time

Group Display commands

Syntax DISPlay:IQVTime:Y[:SCALe]:RESCale

Arguments None

Examples DISPLAY:IQVTIME:Y:SCALE:RESCALE rescales the vertical axis automatically to fit the waveform to the screen.

DISPlay:MCPower:MARKer:SHOW:STATE

Determines whether to show or hide the readout for the selected marker in the MCPR view.

Conditions	Measurement views: MCPR
Group	Display commands
Syntax	DISP <code>l</code> ay:MCPower:MARKer:SHOW:STATE { OFF ON 0 1 } DISP <code>l</code> ay:MCPower:MARKer:SHOW:STATE?
Arguments	OFF or 0 hides the readout for the selected marker in the graph. ON or 1 shows the readout for the selected marker in the graph.
Examples	DISP <code>l</code> AY:MCPOWER:MARKER:SHOW:STATE ON shows the readout for the selected marker in the graph.

DISP`l`ay:MCPower:PLEV`l`:SHOW:STATE

Determines whether to show or hide the power levels in the MCPR view.

Conditions	Measurement views: MCPR
Group	Display commands
Syntax	DISP <code>l</code> ay:MCPower:PLEV <code>l</code> :SHOW:STATE { OFF ON 0 1 } DISP <code>l</code> ay:MCPower:PLEV <code>l</code> :SHOW:STATE?
Arguments	OFF or 0 hides the power levels in the graph. ON or 1 shows the power levels in the graph.
Examples	DISP <code>l</code> AY:MCPOWER:PLEVEL:SHOW:STATE ON shows the power levels in the graph.

DISPlay:MCPower:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the MCPR view.

Vertical offset = Reference level,
Vertical scale = 100 dB,
Horizontal offset = Center frequency, and
Horizontal scale = Default span

Conditions	Measurement views: MCPR
Group	Display commands
Syntax	DISPlay:MCPower:RESet:SCALE
Arguments	None
Examples	DISPLAY:MCPOWER:RESET:SCALE resets the horizontal and vertical scale to the default values.

DISPlay:MCPower:WINDow:TRACe:GRATICule:GRID:STATE

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: MCPR
Group	Display commands
Syntax	DISPlay:MCPower:WINDow:TRACe:GRATICule:GRID:STATE { OFF ON 0 1 } DISPlay:MCPower:WINDow:TRACe:GRATICule:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPLAY:MCPOWER:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen.

DISPlay:MCPower:X[:SCALE]

Sets or queries the horizontal range of the MCPR graph.

Conditions Measurement views: MCPR

Group Display commands

Syntax DISPlay:MCPower:X[:SCALE] <value>
DISPlay:MCPower:X[:SCALE]?

Related Commands [DISPlay:MCPower:X\[:SCALE\]:OFFSet](#)

Arguments <value>::=<Nrf> specifies the horizontal range.
Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples DISPLAY:MCPOWER:X:SCALE 10MHZ sets the horizontal range to 10 MHz.

DISPlay:MCPower:X[:SCALE]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the MCPR view.

Conditions Measurement views: MCPR

Group Display commands

Syntax DISPlay:MCPower:X[:SCALE]:AUTO

Arguments None

Examples DISPLAY:MCPOWER:X:SCALE:AUTO rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:MCPower:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the MCPR graph.

Conditions Measurement views: MCPR

Group Display commands

Syntax `DISPlay:MCPower:X[:SCALE]:OFFSet <value>`
`DISPlay:MCPower:X[:SCALE]:OFFSet?`

Related Commands [DISPlay:MCPower:X\[:SCALE\]](#)

Arguments `<value> ::= <NRF>` specifies the minimum horizontal value.
 Range: $[(\text{center frequency}) - (\text{X scale}) \times 0.9]$ to $[(\text{center frequency}) + (\text{X scale}) \times 0.9]$

Examples `DISPlay:MCPOWER:X:SCALE:OFFSet 1.45GHZ` sets the minimum horizontal value to 1.45 GHz in the MCPR graph.

DISPlay:MCPower:Y[:SCALE]

Sets or queries the vertical range of the MCPR graph.

Conditions Measurement views: MCPR

Group Display commands

Syntax `DISPlay:MCPower:Y[:SCALE] <value>`
`DISPlay:MCPower:Y[:SCALE]?`

Related Commands [DISPlay:MCPower:Y\[:SCALE\]:OFFSet](#)

Arguments `<value> ::= <NRF>` specifies the vertical range. Range: 0.1 to 200 dB.

Examples `DISPlay:MCPOWER:Y:SCALE 100` sets the vertical range to 100 dB in the MCPR graph.

DISPlay:MCPower:Y[:SCALE]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the MCPR view.

Conditions Measurement views: MCPR

Group Display commands

Syntax DISPlay:MCPower:Y[:SCALE]:AUTO

Arguments None

Examples DISPLAY:MCPOWER:Y:SCALE:AUTO rescales the vertical scale automatically to fit the waveform to the screen.

DISPlay:MCPower:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the MCPR graph.

Conditions Measurement views: MCPR

Group Display commands

Syntax DISPlay:MCPower:Y[:SCALE]:OFFSet <value>
DISPlay:MCPower:Y[:SCALE]:OFFSet?

Related Commands [DISPlay:MCPower:Y\[:SCALE\]](#)

Arguments <value>::=<NRF> specifies the vertical offset. Range: -170 to +50 dBm.

Examples DISPLAY:MCPOWER:Y:SCALE:OFFSET -12.5 sets the vertical offset to -12.5 dBm in the MCPR graph.

DISPlay:MERRor:WINDow:TRACe:GRATICule:GRID:STATe

Sets or queries the graticule grid view state for the Magnitude Error versus Time view.

Conditions	Measurement views: Magnitude error versus Time
Group	Display commands
Syntax	DISPlay:MERRor:WINDow:TRACe:GRATICule:GRID:STATe { OFF ON 0 1 } DISPlay:MERRor:WINDow:TRACe:GRATICule:GRID:STATe?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPlay:MERRor:WINDow:TRACe:GRATICule:GRID:STATe ON shows the graticule grid on the Magnitude Error versus Time view.

DISPlay:MERRor:Y[:SCALe]

Sets or queries the vertical range of the Magnitude Error versus Time graph.

Conditions	Measurement views: Magnitude Error versus Time
Group	Display commands
Syntax	DISPlay:MERRor:Y[:SCALe] <value> DISPlay:MERRor:Y[:SCALe]?
Related Commands	DISPlay:MERRor:Y[:SCALe]:OFFSet
Arguments	<value> ::= <Nrf> specifies the vertical range. Range: 1 to 100%.
Examples	DISPlay:MERRor:Y:SCALe 50 sets the vertical range to 50% in the Magnitude error versus Time graph.

DISPlay:MERRor:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Magnitude error versus Time view.

Conditions Measurement views: Magnitude error versus Time

Group Display commands

Syntax DISPlay:MERRor:Y[:SCALE]:AUTO

Arguments None

Examples DISPLAY:MERROR:Y:SCALE:AUTO sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:MERRor:Y[:SCALE]:OFFSet

Sets or queries the minimum vertical value (bottom edge) of the Magnitude error versus Time graph.

Conditions Measurement views: Magnitude error versus Time

Group Display commands

Syntax DISPlay:MERRor:Y[:SCALE]:OFFSet <value>
DISPlay:MERRor:Y[:SCALE]:OFFSet?

Related Commands [DISPlay:MERRor:Y\[:SCALE\]](#)

Arguments <value>::=<NRF> specifies the minimum vertical value. Range: -100 to +100%.

Examples DISPLAY:MERROR:Y:SCALE:OFFSET -9.5 sets the minimum vertical value to -9.5% in the Magnitude error versus Time graph.

DISPlay:OBWidth:MARKer:SHOW:STATe

Determines whether to show or hide the readout for the selected marker in the Occupied Bandwidth view.

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBwidth:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
DISPlay:OBwidth:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the readout for the selected marker in the view.
ON or 1 shows the readout for the selected marker in the view.

Examples DISPLAY:OBWIDTH:MARKER:SHOW:STATE ON shows the readout for the selected marker in the view.

DISPlay:OBWidth:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the Occupied Bandwidth view.

Vertical offset = Reference level,
Vertical scale = 100 dB,
Horizontal offset = Center frequency, and
Horizontal scale = Default span

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBwidth:RESet:SCALE

Arguments None

Examples DISPLAY:OBWIDTH:RESET:SCALE resets the horizontal and vertical scale to the default values.

DISPlay:OBWidth:SElected:BANDwidth

Sets or queries the bandwidth (OBW or x dB BW) to measure in the Occupied Bandwidth view.

Conditions	Measurement views: Occupied Bandwidth
Group	Display commands
Syntax	DISPlay:OBwidth:SElected:BANDwidth { OBwidth XDBbandwidth } DISPlay:OBwidth:SElected:BANDwidth?
Arguments	OBwidth selects the occupied bandwidth to measure. XDBbandwidth selects the x dB bandwidth to measure.
Examples	DISPLAY:OBWIDTH:SELECTED:BANDWIDTH OBwidth selects the occupied bandwidth to measure.

DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATE

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Occupied Bandwidth
Group	Display commands
Syntax	DISPlay:OBwidth:WINDow:TRACe:GRATicule:GRID:STATE { OFF ON 0 1 } DISPlay:OBwidth:WINDow:TRACe:GRATicule:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPLAY:OBWIDTH:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen.

DISPlay:OBWidth:X[:SCALE]

Sets or queries the horizontal range of the Occupied Bandwidth view.

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBWidth:X[:SCALE] <value>
DISPlay:OBWidth:X[:SCALE]?

Related Commands [DISPlay:OBWidth:X\[:SCALE\]:OFFSet](#)

Arguments <value> ::= <Nrf> specifies the horizontal range.
Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples DISPLAY:OBWIDTH:X:SCALE 10MHZ sets the horizontal range to 10 MHz.

DISPlay:OBWidth:X[:SCALE]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the Occupied Bandwidth view.

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBWidth:X[:SCALE]:AUTO

Arguments None

Examples DISPLAY:OBWIDTH:X:SCALE:AUTO rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:OBWidth:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the Occupied Bandwidth view.

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBwidth:X[:SCALE]:OFFSet <value>
DISPlay:OBwidth:X[:SCALE]:OFFSet?

Related Commands [DISPlay:OBWidth:X\[:SCALE\]](#)

Arguments <value>::=<NRF> specifies the minimum horizontal value.
Range: [(center frequency) - (X scale) × 0.9] to [(center frequency) + (X scale) × 0.9]

Examples DISPLAY:OBWIDTH:X:SCALE:OFFSET 1.45GHZ sets the minimum horizontal value to 1.45 GHz in the Occupied Bandwidth view.

DISPlay:OBWidth:Y[:SCALE]

Sets or queries the vertical range of the Occupied Bandwidth view.

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBwidth:Y[:SCALE] <value>
DISPlay:OBwidth:Y[:SCALE]?

Related Commands [DISPlay:OBWidth:Y\[:SCALE\]:OFFSet](#)

Arguments <value>::=<NRF> specifies the vertical range. Range: 0.1 to 200 dB.

Examples DISPLAY:OBWIDTH:Y:SCALE 100 sets the vertical range to 100 dB in the Occupied Bandwidth view.

DISPlay:OBWidth:Y[:SCALE]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Occupied Bandwidth view.

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBWidth:Y[:SCALE]:AUTO

Arguments None

Examples DISPLAY:OBWIDTH:Y:SCALE:AUTO rescales the vertical scale automatically to fit the waveform to the screen.

DISPlay:OBWidth:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the Occupied Bandwidth view.

Conditions Measurement views: Occupied Bandwidth

Group Display commands

Syntax DISPlay:OBWidth:Y[:SCALE]:OFFSet <value>
DISPlay:OBWidth:Y[:SCALE]:OFFSet?

Related Commands [DISPlay:OBWidth:Y\[:SCALE\]](#)

Arguments <value>::=<NRf> specifies the vertical offset. Range: -170 to +50 dBm.

Examples DISPLAY:OBWIDTH:Y:SCALE:OFFSET -12.5 sets the vertical offset to -12.5 dBm in the Occupied Bandwidth view.

DISPlay:PERRor:WINDow:TRACe:GRATICule:GRID:STATE

Sets or queries the graticule grid view state for the Phase error versus Time view.

Conditions	Measurement views: Magnitude error versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:PERRor:WINDow:TRACe:GRATICule:GRID:STATE { OFF ON 0 1 } DISP <code>l</code> ay:PERRor:WINDow:TRACe:GRATICule:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISP <code>l</code> AY:PERRor:WINDow:TRACe:GRATICule:GRID:STATE ON shows the graticule grid on the Phase error versus Time view.

DISP`l`ay:PERRor:Y[:SCALE]

Sets or queries the vertical range of the Phase error versus Time graph.

Conditions	Measurement views: Phase error versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:PERRor:Y[:SCALE] <value> DISP <code>l</code> ay:PERRor:Y[:SCALE]?
Related Commands	DISP<code>l</code>ay:PERRor:Y[:SCALE]:OFFSet
Arguments	<value>::=<NRF> specifies the vertical range. Range: 1 to 360°.
Examples	DISP <code>l</code> AY:PERRor:Y:SCALE 30 sets the vertical range to 30 ° in the Phase error versus Time graph.

DISPlay:PERRor:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Phase error versus Time view.

Conditions Measurement views: Phase error versus Time

Group Display commands

Syntax DISPlay:PERRor:Y[:SCALE]:AUTO

Arguments None

Examples DISPLAY:PERROR:Y:SCALE:AUTO sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:PERRor:Y[:SCALE]:OFFSet

Sets or queries the minimum vertical value (bottom edge) of the Phase error versus Time graph.

Conditions Measurement views: Phase error versus Time

Group Display commands

Syntax DISPlay:PERRor:Y[:SCALE]:OFFSet <value>
DISPlay:PERRor:Y[:SCALE]:OFFSet?

Related Commands [DISPlay:PERRor:Y\[:SCALE\]](#)

Arguments <value>::=<NRF> specifies the minimum vertical value. Range: -360 to +360°.

Examples DISPLAY:PERROR:Y:SCALE:OFFSET -14.5 sets the minimum vertical value to -14.5 ° in the Phase Error versus Time graph.

DISPlay:PHVTime:WINDow:TRACe:GRATICule:GRID:STATE

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISPlay:PHVTime:WINDow:TRACe:GRATICule:GRID:STATE { OFF ON 0 1 } DISPlay:PHVTime:WINDow:TRACe:GRATICule:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPLAY:PHVTIME:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the Frequency versus Time view.

DISPlay:PHVTime:X[:SCALE]

Sets or queries the horizontal scale (full-scale time) of the Phase versus Time graph. Programming a specified scale sets DISPlay:PHVTime:X[:SCALE] AUTO:STATE OFF.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISPlay:PHVTime:X[:SCALE] <value> DISPlay:PHVTime:X[:SCALE]?
Related Commands	DISPlay:PHVTime:X[:SCALE]:AUTO:STATE , DISPlay:PHVTime:X[:SCALE]:OFFSET
Arguments	<value>::={ <NRF> MAXimum MINimum } specifies the horizontal scale in full-scale time. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.

Use the [DISPlay:PHVTime:X\[:SCALe\]:MAXimum?](#) and [DISPlay:PHVTime:X\[:SCALe\]:OFFSet:MINimum?](#) queries to get the upper and lower limit values of the setting range.

Examples `DISPLAY:PHVTIME:X:SCALE 1.5ms` sets the horizontal scale to 1.5 ms.

DISPlay:PHVTime:X[:SCALe]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the Phase versus Time view. Executing this command sets `DISPlay:PHVTime:X[:SCALe]:AUTO:STATe ON`.

Conditions Measurement views: Phase versus Time

Group Display commands

Syntax `DISPlay:PHVTime:X[:SCALe]:AUTO`

Related Commands [DISPlay:PHVTime:X\[:SCALe\]:AUTO:STATe](#)

Arguments None

Examples `DISPLAY:PHVTIME:X:SCALE:AUTO` sets the horizontal scale automatically to fit the waveform to the screen.

DISPlay:PHVTime:X[:SCALe]:AUTO:STATe

Determines whether to set the horizontal scale automatically or manually.

Conditions Measurement views: Phase versus Time

Group Display commands

Syntax `DISPlay:PHVTime:X[:SCALe]:AUTO:STATe { OFF | ON | 0 | 1 }`
`DISPlay:PHVTime:X[:SCALe]:AUTO:STATe?`

Arguments OFF or 0 specifies that the horizontal scale is set manually. To set it, use the [DISPlay:PHVTime:X\[:SCALE\]](#) and [DISPlay:PHVTime:X\[:SCALE\]:OFFSet](#) commands.

ON or 1 specifies that the horizontal scale is set automatically.

Examples `DISPlay:PHVTime:X:SCALE:AUTO:STATE ON` specifies that the horizontal scale is set automatically.

DISPlay:PHVTime:X[:SCALE]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Conditions Measurement views: Phase versus Time

Group Display commands

Syntax `DISPlay:PHVTime:X[:SCALE]:MAXimum?`

Related Commands [DISPlay:PHVTime:X\[:SCALE\]](#)

Arguments None

Returns <NRF> The upper limit of the horizontal scale setting range.

Examples `DISPlay:PHVTime:X:SCALE:MAXIMUM?` might return `18.135E-3`, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

DISPlay:PHVTime:X[:SCALE]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Conditions Measurement views: Phase versus Time

Group Display commands

Syntax `DISPlay:PHVTime:X[:SCALE]:MINimum?`

Related Commands	DISPlay:PHVTime:X[:SCALE]
Arguments	None
Returns	<Nrf> The lower limit of the horizontal scale setting range.
Examples	DISPLAY:PHVTIME:X:SCALE:MINIMUM? might return 10.0E-9, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

DISPlay:PHVTime:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the Phase versus Time graph. Programming a specified offset sets DISPlay:PHVTime:X[:SCALE]:AUTO:STATe OFF.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISPlay:PHVTime:X[:SCALE]:OFFSet DISPlay:PHVTime:X[:SCALE]:OFFSet?
Related Commands	DISPlay:PHVTime:X[:SCALE]:AUTO:STATe , DISPlay:PHVTime:X[:SCALE] ,
Arguments	<p><value>::={ <Nrf> MAXimum MINimum } specifies the horizontal offset. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.</p> <p>Use the DISPlay:PHVTime:X[:SCALE]:OFFSet:MAXimum? and DISPlay:PHVTime:X[:SCALE]:OFFSet:MINimum? queries to get the upper and lower limit values of the setting range.</p>
Examples	DISPLAY:PHVTIME:X:SCALE:OFFSET 800ns sets the minimum horizontal value to 800 ns in the Phase versus Time graph.

DISPlay:PHVTime:X[:SCALE]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:PHVTime:X[:SCALE]:OFFSet:MAXimum?
Related Commands	DISP<code>l</code>ay:PHVTime:X[:SCALE]:OFFSet
Arguments	None
Returns	<NRf> The upper limit of the horizontal offset setting range.
Examples	DISP <code>l</code> ay:PHVTime:X:SCALE:OFFSet:MAXIMUM? might return $-1.812E-3$, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

DISP`l`ay:PHVTime:X[:SCALE]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISP <code>l</code> ay:PHVTime:X[:SCALE]:OFFSet:MINimum?
Related Commands	DISP<code>l</code>ay:PHVTime:X[:SCALE]:OFFSet
Arguments	None
Returns	<NRf> The lower limit of the horizontal offset setting range.
Examples	DISP <code>l</code> ay:PHVTime:X:SCALE:OFFSet:MINIMUM? might return $-16.28E-3$, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

DISPlay:PHVTime:Y[:SCALe]

Sets or queries the vertical range of the Phase versus Time graph.

Conditions Measurement views: Phase versus Time

Group Display commands

Syntax DISPlay:PHVTime:Y[:SCALe] <value>
DISPlay:PHVTime:Y[:SCALe]?

Related Commands [DISPlay:PHVTime:Y\[:SCALe\]:OFFSet](#)

Arguments <value>::=<Nrf> specifies the vertical range. Range: 1 to 1T °.

Examples DISPLAY:PHVTIME:Y:SCALE 180 sets the vertical range to 180 ° in the Phase versus Time graph.

DISPlay:PHVTime:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Phase versus Time view.

Conditions Measurement views: Phase versus Time

Group Display commands

Syntax DISPlay:PHVTime:Y[:SCALe]:AUTO

Arguments None

Examples DISPLAY:PHVTIME:Y:SCALE:AUTO sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:PHVTime:Y[:SCALe]:AXIS

Sets or queries the vertical axis representation.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISPlay:PHVTime:Y[:SCALE]:AXIS { MODulo π CONTinuous } DISPlay:PHVTime:Y[:SCALE]:AXIS?
Arguments	MODulo π (modulo π) shows the phase constrained within $\pm 180^\circ$ along the vertical axis. CONTinuous shows the phase as continuous quantity along the vertical axis.
Examples	DISPLAY:PHVTIME:Y:SCALE:AXIS MODulo π selects modulo π representation for the vertical axis.

DISPlay:PHVTime:Y[:SCALE]:AXIS:REFerence

Sets or queries which time point in the analysis period to use as the zero-phase-value reference.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISPlay:PHVTime:Y[:SCALE]:AXIS:REFerence <value> DISPlay:PHVTime:Y[:SCALE]:AXIS:REFerence?
Arguments	<value>::=<NRF> specifies the phase reference time.
Examples	DISPLAY:PHVTIME:Y:SCALE:AXIS:REFERENCE 1.5us sets the phase reference time to 1.5 μ s.

DISPlay:PHVTime:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the center of the vertical axis) in the Phase versus Time graph.

Conditions	Measurement views: Phase versus Time
-------------------	--------------------------------------

Group	Display commands
Syntax	DISPlay:PHVTime:Y[:SCALE]:OFFSet <value> DISPlay:PHVTime:Y[:SCALE]:OFFSet?
Related Commands	DISPlay:PHVTime:Y[:SCALE]
Arguments	<value>::=<Nrf> specifies the vertical offset. Range: -0.5T to +0.5T°.
Examples	DISPLAY:PHVTIME:Y:SCALE:OFFSET -158.5 sets the vertical offset to -158.5° in the Phase versus Time graph.

DISPlay:PHVTime:Y[:SCALE]:RESCale (No Query Form)

Rescales the vertical axis automatically to fit the Phase versus Time waveform to the screen.

Conditions	Measurement views: Phase versus Time
Group	Display commands
Syntax	DISPlay:PHVTime:Y[:SCALE]:RESCale
Arguments	None
Examples	DISPLAY:PHVTIME:Y:SCALE:RESCALE rescales the vertical axis automatically to fit the Phase versus Time waveform to the screen.

DISPlay:PNOise:LEGend:STATe

Determines whether to show or hide the trace legend on the display. The legend indicates the trace detection and function on the screen for each displayed trace.

Conditions	Measurement views: Phase versus Time
Group	Display commands

Syntax `DISPlay:PNOise:LEGenD:STATe { OFF | ON | 0 | 1 }`
`DISPlay:PNOise:LEGenD:STATe?`

Arguments OFF or 0 hides the trace legend.
 ON or 1 shows the trace legend.

Examples `DISPlay:PNOise:LEGenD:STATe ON` shows the trace legend on the screen.

DISPlay:PNOise:MARKer:SHOW:STATE

Determines whether to show or hide the readout for the selected marker in the phase noise view.

Conditions Measurement views: Phase noise

Group Display commands

Syntax `DISPlay:PNOise:MARKer:SHOW:STATE { OFF | ON | 0 | 1 }`
`DISPlay:PNOise:MARKer:SHOW:STATE?`

Arguments OFF or 0 hides the readout for the selected marker in the graph.
 ON or 1 shows the readout for the selected marker in the graph.

Examples `DISPlay:PNOise:MARKer:SHOW:STATE ON` shows the readout for the selected marker in the graph.

DISPlay:PNOise:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the phase noise view.

Vertical offset = -50 dBc/Hz,
 Vertical scale = 100 dB,
 Horizontal start = 10 Hz, and
 Horizontal stop = 1 GHz

Conditions Measurement views: Phase noise

Group	Display commands
Syntax	DISP <code>l</code> ay:PNOi <code>s</code> e:RESE <code>t</code> :SCAL <code>e</code>
Arguments	None
Examples	DISP <code>l</code> ay:PNOI <code>S</code> E:RESE <code>T</code> :SCAL <code>E</code> resets the horizontal and vertical scale to the default values.

DISP`l`ay:PNOi`s`e:WINDow:TRACe:GRATi`c`ule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Phase noise
Group	Display commands
Syntax	DISP <code>l</code> ay:PNOi <code>s</code> e:WINDow:TRACe:GRATi <code>c</code> ule:GRID:STATe { OFF ON 0 1 } DISP <code>l</code> ay:PNOi <code>s</code> e:WINDow:TRACe:GRATi <code>c</code> ule:GRID:STATe?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISP <code>l</code> ay:PNOI <code>S</code> E:WINDow:TRACe:GRATICULE:GRID:STATe ON shows the graticule grid on the screen.

DISP`l`ay:PNOi`s`e:X[:SCALe]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the phase noise view.

Conditions	Measurement views: Phase noise
Group	Display commands

Syntax `DISPlay:PNOise:X[:SCALE]:AUTO`

Arguments None

Examples `DISPLAY:PNOISE:X:SCALE:AUTO` rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:PNOise:X[:SCALE]:START

Sets or queries the start frequency (left edge) of the phase noise graph.

Conditions Measurement views: Phase noise

Group Display commands

Syntax `DISPlay:PNOise:X[:SCALE]:START <value>`
`DISPlay:PNOise:X[:SCALE]:START?`

Arguments `<value>::=<Nrf>` specifies the start frequency.
 Range: 10 mHz to 100 MHz.
 Note that (start frequency) = $10^4 \times$ (stop frequency).

Examples `DISPLAY:PNOISE:X:SCALE:START 10Hz` sets the start frequency to 10 Hz in the phase noise graph.

DISPlay:PNOise:X[:SCALE]:STOP

Sets or queries the stop frequency (right edge) of the phase noise graph.

Conditions Measurement views: Phase noise

Group Display commands

Syntax `DISPlay:PNOise:X[:SCALE]:STOP <value>`
`DISPlay:PNOise:X[:SCALE]:STOP?`

Arguments <value>::=<Nrf> specifies the stop frequency.
Range: 100 Hz to 1 THz.
Note that (start frequency) = $10^4 \times$ (stop frequency).

Examples DISPLAY:PNOISE:X:SCALE:STOP 2GHZ sets the stop frequency to 2 GHz in the phase noise graph.

DISPlay:PNOise:Y[:SCALe]

Sets or queries the vertical range of the phase noise graph.

Conditions Measurement views: Phase noise

Group Display commands

Syntax DISPlay:PNOise:Y[:SCALe] <value>
DISPlay:PNOise:Y[:SCALe]?

Arguments <value>::=<Nrf> specifies the vertical range. Range: 0.1 to 200 dB.

Examples DISPLAY:PNOISE:Y:SCALE 100 sets the vertical range to 100 dB for the phase noise graph.

DISPlay:PNOise:Y[:SCALe]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the phase noise view.

Conditions Measurement views: Phase noise

Group Display commands

Syntax DISPlay:PNOise:Y[:SCALe]:AUTO

Arguments None

Examples `DISPLAY:PNOISE:Y:SCALE:AUTO` rescales the vertical scale automatically to fit the waveform to the screen.

DISPlay:PNOise:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) of the phase noise graph.

Conditions Measurement views: Phase noise

Group Display commands

Syntax `DISPlay:PNOise:Y[:SCALE]:OFFSet <value>`
`DISPlay:PNOise:Y[:SCALE]:OFFSet?`

Arguments `<value>::=<NRF>` specifies the vertical offset. Range: -200 to +20 dBc/Hz.

Examples `DISPLAY:PNOISE:Y:SCALE:OFFSET -12.5` sets the vertical offset to -12.5 dBc/Hz for the phase noise graph.

DISPlay:PNOise:Y[:SCALE]:PDIVision

Sets or queries the vertical scale (per division) of the phase noise graph.

Conditions Measurement views: Phase noise

Group Display commands

Syntax `DISPlay:PNOise:Y[:SCALE]:PDIVision <value>`
`DISPlay:PNOise:Y[:SCALE]:PDIVision?`

Arguments `<value>::=<NRF>` specifies the vertical scale (per division).
 Range: 0.01 to 20 dB/div.

Examples `DISPLAY:PNOISE:Y:SCALE:PDIVISION 5` sets the vertical scale to 5 dB/div.

DISPlay:PULSe:MEASview:DELeTe (No Query Form)

Deletes the measurement view in the pulsed RF measurements.

Conditions Measurement views: Pulsed RF measurements

Group Display commands

Syntax DISPlay:PULSe:MEASview:DELeTe { RESuLt | TRACe | STATistics }
}

Arguments RESuLt deletes the pulse table view.
TRACe deletes the pulse trace view.
STATistics deletes the pulse statistics view.
If you attempt to delete a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Examples DISPLAY:PULSE:MEASVIEW:DELETE TRACe deletes the pulse trace view.

DISPlay:PULSe:MEASview:NEW (No Query Form)

Displays a new measurement view in the pulsed RF measurements.

Conditions Measurement views: Pulsed RF measurements

Group Display commands

Syntax DISPlay:PULSe:MEASview:NEW { RESuLt | TRACe | STATistics }
}

Arguments RESuLt opens the pulse table view.
TRACe opens the pulse trace view.
STATistics opens the pulse statistics view.
If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.

Examples `DISPLAY:PULSE:MEASVIEW:NEW STATISTICS` creates the pulse statistics view.

DISPlay:PULSe:MEASview:SElect

Selects a measurement view in the pulsed RF measurements on the screen. The query command returns the currently selected view.

Conditions Measurement views: Pulsed RF measurements

Group Display commands

Syntax `DISPlay:PULSe:MEASview:SElect { RESuLt | TRACe | STATISTICS }`
`DISPlay:PULSe:MEASview:SElect?`

Arguments `RESuLt` selects the pulse table view.
`TRACe` selects the pulse trace view.
`STATISTICS` selects the pulse statistics view.
 If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Examples `DISPLAY:PULSE:MEASVIEW:SELECT TRACe` selects the pulse trace view.

DISPlay:PULSe:RESuLt:ATX

Determines whether or not to show the average transmitted power measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPlay:PULSe:RESuLt:ATX { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:RESuLt:ATX?`

Arguments OFF or 0 does not show the average transmitted power measurement result.
ON or 1 shows the average transmitted power measurement result in the pulse table.

Examples DISPLAY:PULSE:RESULT:ATX ON shows the average transmitted power measurement result in the pulse table.

DISPlay:PULSe:RESuLt:AVERAge

Determines whether or not to show the average on power measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESuLt:AVERAge { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:AVERAge?

Arguments OFF or 0 does not show the average on power measurement result.
ON or 1 shows the average on power measurement result in the results table.

Examples DISPLAY:PULSE:RESULT:AVERAGE ON shows the average on power measurement result in the pulse table.

DISPlay:PULSe:RESuLt:DRODb

Determines whether or not to show the droop measurement result in dB in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESuLt:DRODb { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:DRODb?

Arguments OFF or 0 does not show the droop measurement result in dB.
ON or 1 shows the droop measurement result in dB in the pulse table.

Examples DISPLAY:PULSE:RESULT:DRODB ON shows the droop measurement result in dB in the pulse table.

DISPlay:PULSe:RESuLt:DROop

Sets or queries showing the droop measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESuLt:DROop { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:DROop?

Arguments OFF or 0 does not show the droop measurement result.
ON or 1 shows the droop measurement result in the pulse table.

Examples DISPLAY:PULSE:RESULT:DROOP ON shows the droop measurement result in the pulse table.

DISPlay:PULSe:RESuLt:DUTPct

Determines whether or not to show the duty factor (%) measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESuLt:DUTPct { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:DUTPct?

- Arguments** OFF or 0 does not show the duty factor measurement result.
ON or 1 shows the duty factor measurement result in the pulse table.
- Examples** DISPLAY:PULSE:RESULT:DUTPCT ON shows the duty factor (%) measurement result in the pulse table.

DISPlay:PULSe:RESuLt:DUTRatio

Determines whether or not to show the duty factor (ratio) measurement result in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** DISPlay:PULSe:RESuLt:DUTRatio { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:DUTRatio?
- Arguments** OFF or 0 does not show the duty factor measurement result.
ON or 1 shows the duty factor measurement result in the pulse table.
- Examples** DISPLAY:PULSE:RESULT:DUTRATIO ON shows the duty factor (ratio) measurement result in the pulse table.

DISPlay:PULSe:RESuLt:FALL

Determines whether or not to show the fall time measurement result in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** DISPlay:PULSe:RESuLt:FALL { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:FALL?

Arguments OFF or 0 does not show the fall time measurement result.
ON or 1 shows the fall time measurement result in the pulse table.

Examples DISPLAY:PULSE:RESULT:FALL ON shows the fall time measurement result in the pulse table.

DISPlay:PULSe:RESult:FRDeviation

Determines whether or not to show the frequency deviation measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESult:FRDeviation { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESult:FRDeviation?

Arguments OFF or 0 does not show the frequency deviation measurement result.
ON or 1 shows the frequency deviation measurement result in the pulse table.

Examples DISPLAY:PULSE:RESULT:FRDEVIATION ON shows the frequency deviation measurement result in the pulse table.

DISPlay:PULSe:RESult:IRAMplitude

Sets or queries showing the impulse response amplitude measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESult:IRAMplitude { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESult:IRAMplitude?

Arguments OFF or 0 does not show the Impulse Response Amplitude measurement result.
ON or 1 shows the Impulse Response Amplitude measurement result in the results table.

Examples DISPLAY:PULSE:RESULT:IRAMPLITUDE ON shows the Impulse Response Amplitude measurement result in the pulse table.

DISPlay:PULSe:RESult:IRTime

Sets or queries showing the Impulse Response Time measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESult:IRTime { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESult:IRTime?

Arguments OFF or 0 does not show the Impulse Response Time measurement result.
ON or 1 shows the Impulse Response Time measurement result in the results table.

Examples DISPLAY:PULSE:RESULT:IRTIME ON shows the Impulse Response Time measurement result in the pulse table.

DISPlay:PULSe:RESult:MFRreqerror

Determines whether or not to show the maximum frequency error measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESult:MFRreqerror { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESult:MFRreqerror?

- Arguments** OFF or 0 does not show the maximum frequency error measurement result.
ON or 1 shows the maximum frequency error measurement result in the pulse table.
- Examples** DISPLAY:PULSE:RESULT:MFREQERROR ON shows the maximum frequency error measurement result in the pulse table.

DISPlay:PULSe:RESult:MPHerror

Determines whether or not to show the maximum phase error measurement result in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** DISPlay:PULSe:RESuIt:MPHerror { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuIt:MPHerror?
- Arguments** OFF or 0 does not show the maximum phase error measurement result.
ON or 1 shows the maximum phase error measurement result in the pulse table.
- Examples** DISPLAY:PULSE:RESULT:MPHERROR ON shows the maximum phase error measurement result in the pulse table.

DISPlay:PULSe:RESult:OVEDb

Determines whether or not to show the Overshoot measurement result in dB in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** DISPlay:PULSe:RESuIt:OVEDb { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuIt:OVEDb?

- Arguments** OFF or 0 does not show the Overshoot measurement result in dB.
ON or 1 shows the Overshoot measurement result in dB in the pulse table.
- Examples** `DISPlay:PULSe:RESuLt:OVEDB ON` shows the Overshoot measurement result in dB in the pulse table.

DISPlay:PULSe:RESuLt:OVERshoot

Sets or queries whether or not to show the Overshoot measurement result in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** `DISPlay:PULSe:RESuLt:OVERshoot { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:RESuLt:OVERshoot?`
- Arguments** OFF or 0 does not show the Overshoot measurement result.
ON or 1 shows the Overshoot measurement result in the pulse table.
- Examples** `DISPlay:PULSe:RESuLt:OVERSHOOT ON` shows the Overshoot measurement result in the pulse table.

DISPlay:PULSe:RESuLt:PHDeviation

Determines whether or not to show the phase deviation measurement result in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** `DISPlay:PULSe:RESuLt:PHDeviation { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:RESuLt:PHDeviation?`

- Arguments** OFF or 0 does not show the phase deviation measurement result.
ON or 1 shows the phase deviation measurement result in the pulse table.
- Examples** DISPLAY:PULSE:RESULT:PHDEVIATION ON shows the phase deviation measurement result in the pulse table.

DISPlay:PULSe:RESuLt:PPFRequency

Determines whether or not to show the pulse-pulse carrier frequency measurement result in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** DISPlay:PULSe:RESuLt:PPFRequency { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:PPFRequency?
- Arguments** OFF or 0 does not show the pulse-pulse carrier frequency measurement result.
ON or 1 shows the pulse-pulse carrier frequency measurement result in the pulse table.
- Examples** DISPLAY:PULSE:RESULT:PPFREQUENCY ON shows the pulse-pulse carrier frequency measurement result in the pulse table.

DISPlay:PULSe:RESuLt:PPOWer

Determines whether or not to show the peak power measurement result in the pulse table.

- Conditions** Measurement views: Pulse table
- Group** Display commands
- Syntax** DISPlay:PULSe:RESuLt:PPOWer { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:PPOWer?

Arguments OFF or 0 does not show the peak power measurement result.
ON or 1 shows the peak power measurement result in the pulse table.

Examples DISPLAY:PULSE:RESULT:PPOWER ON shows the peak power measurement result in the pulse table.

DISPlay:PULSe:RESuLt:PPHase

Determines whether or not to show the pulse-pulse carrier phase measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESuLt:PPHase { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:PPHase?

Arguments OFF or 0 does not show the pulse-pulse carrier phase measurement result.
ON or 1 shows the pulse-pulse carrier phase measurement result in the pulse table.

Examples DISPLAY:PULSE:RESULT:PPHASE ON shows the pulse-pulse carrier phase measurement result in the pulse table.

DISPlay:PULSe:RESuLt:RINterval

Determines whether or not to show the repetition interval measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax DISPlay:PULSe:RESuLt:RINterval { OFF | ON | 0 | 1 }
DISPlay:PULSe:RESuLt:RINterval?

Arguments OFF or 0 does not show the repetition interval measurement result.
ON or 1 shows the repetition interval measurement result in the results table.

Examples `DISPLAY:PULSE:RESULT:RINTERVAL ON` shows the repetition interval measurement result in the pulse table.

DISPlay:PULSe:RESuLt:RIPDb

Sets or queries showing the ripple measurement result in dB in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPly:PULSe:RESuLt:RIPDb { OFF | ON | 0 | 1 }`
`DISPly:PULSe:RESuLt:RIPDb?`

Arguments OFF or 0 does not show the ripple measurement result in dB.
ON or 1 shows the ripple measurement result in dB in the pulse table.

Examples `DISPLAY:PULSE:RESULT:RIPDB ON` shows the ripple measurement result in dB in the pulse table.

DISPlay:PULSe:RESuLt:RIPPlE

Sets or queries showing the ripple measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPly:PULSe:RESuLt:RIPPlE { OFF | ON | 0 | 1 }`
`DISPly:PULSe:RESuLt:RIPPlE?`

Arguments OFF or 0 does not show the ripple measurement result.
ON or 1 shows the ripple measurement result in the pulse table.

Examples `DISPLAY:PULSE:RESULT:RIPPLE ON` shows the ripple measurement result in the pulse table.

DISPlay:PULSe:RESuLt:RISE

Determines whether or not to show the rise time measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPlay:PULSe:RESuLt:RISE { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:RESuLt:RISE?`

Arguments OFF or 0 does not show the rise time measurement result.
ON or 1 shows the rise time measurement result in the pulse table.

Examples `DISPLAY:PULSE:RESULT:RISE ON` shows the rise time measurement result in the pulse table.

DISPlay:PULSe:RESuLt:RMSFreqerror

Determines whether or not to show the RMS frequency error measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPlay:PULSe:RESuLt:RMSFreqerror { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:RESuLt:RMSFreqerror?`

Arguments OFF or 0 does not show the RMS frequency error measurement result.
ON or 1 shows the RMS frequency error measurement result in the pulse table.

Examples `DISPLAY:PULSE:RESULT:RMSFREQERROR ON` shows the RMS frequency error measurement result in the pulse table.

DISPlay:PULSe:RESuLt:RMSPHerror

Determines whether or not to show the RMS phase error measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPly:PULSe:RESuLt:RMSPHerror { OFF | ON | 0 | 1 }`
`DISPly:PULSe:RESuLt:RMSPHerror?`

Arguments OFF or 0 does not show the RMS phase error measurement result.
ON or 1 shows the RMS phase error measurement result in the pulse table.

Examples `DISPLAY:PULSE:RESULT:RMSPHERROR ON` shows the RMS phase error measurement result in the pulse table.

DISPly:PULSe:RESuLt:RRATe

Determines whether or not to show the repetition rate measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPly:PULSe:RESuLt:RRATe { OFF | ON | 0 | 1 }`
`DISPly:PULSe:RESuLt:RRATe?`

Arguments OFF or 0 does not show the repetition rate measurement result.
ON or 1 shows the repetition rate measurement result in the pulse table.

Examples `DISPLAY:PULSE:RESULT:RRATE ON` shows the repetition rate measurement result in the pulse table.

DISPlay:PULSe:RESUlt:TIME

Determines whether or not to show the time measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPlay:PULSe:RESUlt:TIME { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:RESUlt:TIME?`

Arguments OFF or 0 does not show the time measurement result.
ON or 1 shows the time measurement result in the pulse table.

Examples `DISPLAY:PULSE:RESULT:TIME ON` shows the time measurement result in the pulse table.

DISPlay:PULSe:RESUlt:WIDTh

Determines whether or not to show the pulse width measurement result in the pulse table.

Conditions Measurement views: Pulse table

Group Display commands

Syntax `DISPlay:PULSe:RESUlt:WIDTh { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:RESUlt:WIDTh?`

Arguments OFF or 0 does not show the pulse width measurement result.
ON or 1 shows the pulse width measurement result in the pulse table.

Examples `DISPLAY:PULSE:RESULT:WIDTH ON` shows the pulse width measurement result in the pulse table.

DISPlay:PULSe:SElect:NUMBER

Sets or queries a pulse to measure. For the selected pulse, the statistics view indicates the measurement result while the table view highlights it, and the trace view displays the waveform.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Display commands

Syntax DISPlay:PULSe:SElect:NUMBER <number>
DISPlay:PULSe:SElect:NUMBER?

Arguments <number>: :=<NR1> specifies the number of pulse to measure.
Range: -(the number of acquired pulses before the time reference) to +(the number of acquired pulses after the time reference).

Zero (0) represents the pulse at the analysis time reference specified using the [\[SENSe\]:ANALysis:REFerence](#) command. The number of acquired pulses depends on the analysis range.

Examples DISPLAY:WINDOW:SELECT:NUMBER -28 measures the pulse #-28.

DISPlay:PULSe:SElect:RESult

Sets or queries which result is shown in the pulse trace and statistics views.

Conditions Measurement views: Pulse statistics, Pulse trace

Group Display commands

Syntax DISPlay:PULSe:SElect:RESult { AVERAge | PPOwer | ATX |
WIDTh | RISE | FALL | RINTerva | RRATe | DUTPct | DUTRatio |
RIPPl | RIPDb | DROop | DRODb | OVERshoot | OVEDb | PPPHase
| PPFRequency | RMSFRequerror | MFRequerror | RMSPherror |
MPHerror | FRDeviation | PHDeviation | IRAMplitude | IRTIME
}
DISPlay:PULSe:SElect:RESult?

Arguments The following table lists the arguments.

Table 2-32: Pulse results

Argument	Result
AVERage	Average on power
PPOWer	Peak power
ATX	Average transmitted power
WIDTh	Pulse width
RISE	Rise time
FALL	Fall time
RINterval	Repetition interval
RRATe	Repetition rate
DUTPct	Duty factor (%)
DUTRatio	Duty factor (ratio)
RIPPlE	Ripple
RIPDb	Ripple (dB)
DROop	Droop
DRODb	Droop (dB)
OVERshoot	Overshoot
OVEDb	Overshoot (dB)
PPPHase	Pulse-pulse carrier phase
PPFRequency	Pulse-pulse carrier frequency
RMSFreqerror	RMS frequency error
MFReqerror	Maximum frequency error
RMSPherror	RMS phase error
MPHerror	Maximum phase error
FRDeviation	Frequency deviation
PHDeviation	Phase deviation
IRAMplitude	Impulse Response Amplitude
IRTime	Impulse Response Sidelobe Offset Time from Mainlobe

Examples `DISPLAY:PULSE:SELECT:RESULT AVERage` shows the average on power result in the pulse trace and statistics views.

DISPlay:PULSe:STATistics:MARKer:SHOW:STATe

Determines whether to show or hide the marker readout in the statistics graph. This command is valid when `DISPlay:PULSe:STATistics:PLOT` is set to FFT.

Conditions	Measurement views: Pulse statistics
Group	Display commands
Syntax	DISP <code>l</code> ay:PULSE:STATISTICS:MARKER:SHOW:STATE { OFF ON 0 1 } DISP <code>l</code> ay:PULSE:STATISTICS:MARKER:SHOW:STATE?
Arguments	OFF or 0 hides the marker readout. ON or 1 shows the marker readout.
Examples	DISP <code>l</code> AY:PULSE:STATISTICS:MARKER:SHOW:STATE ON shows the marker readout in the statistics graph.

DISP`l`ay:PULSE:STATISTICS:PLOT

Sets or queries how to show the statistics graph.

Conditions	Measurement views: Pulse statistics
Group	Display commands
Syntax	DISP <code>l</code> ay:PULSE:STATISTICS:PLOT { TREND FFT TTREnd HISTogram } DISP <code>l</code> ay:PULSE:STATISTICS:PLOT?
Arguments	TREND shows the statistics result along with the pulse number. FFT shows the statistics result transformed into the frequency domain by FFT. TTREnd shows the statistics result along with time. HISTogram shows the histogram statistics results.
Examples	DISP <code>l</code> AY:PULSE:STATISTICS:PLOT TREND shows the statistics result along with the pulse number.

DISPlay:PULSe:STATistics:WINDow:TRACe:GRATICule:GRID:STATe

Determines whether to show or hide the graticule grid in the statistics view.

Conditions	Measurement views: Pulse statistics
Group	Display commands
Syntax	DISPlay:PULSe:STATistics:WINDow:TRACe:GRATICule:GRID:STATe { OFF ON 0 1 } DISPlay:PULSe:STATistics:WINDow:TRACe:GRATICule:GRID:STATe?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPLAY:PULSE:STATISTICS:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the statistics view.

DISPlay:PULSe:STATistics:X:RSCale (No Query Form)

Rescales the horizontal axis to fit the waveform to the screen in the statistics graph.

Conditions	Measurement views: Pulse statistics
Group	Display commands
Syntax	DISPlay:PULSe:STATistics:X:RSCale
Arguments	None
Examples	DISPLAY:PULSE:STATISTICS:X:RSCALE rescales the horizontal axis of the statistics graph.

DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer

Sets or queries the horizontal full scale in the statistics graph.

Conditions Measurement views: Pulse statistics

Group Display commands

Syntax `DISPlay:PULSe:STATistics:X[:SCALE]:NUMBER <value>`
`DISPlay:PULSe:STATistics:X[:SCALE]:NUMBER?`

Related Commands [DISPlay:PULSe:STATistics:X\[:SCALE\]:OFFSet](#)

Arguments `<value>::=<NRF>` specifies the horizontal full scale. The setting range depends on the [DISPlay:PULSe:STATistics:PLOT](#) command parameters as shown in the table below.

<code>DISPlay:PULSe:STATistics:PLOT</code>	Setting range
TREnd	1 to 1000
FFT	1 Hz to 120 MHz

Examples `DISPlay:PULSe:STATistics:X:SCALE:NUMBER 50` sets the horizontal full scale to 50 pulses when the plot is trend.

DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (the first pulse to show) in the statistics graph.

Conditions Measurement views: Pulse statistics

Group Display commands

Syntax `DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet <value>`
`DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet?`

Arguments `<value>::=<NRF>` specifies the number of the first pulse.
 Range: $-(X - X/10)$ to $+(X - X/10)$
 where X is the horizontal scale set by the [DISPlay:PULSe:STATistics:X\[:SCALE\]:NUMBER](#) command.

Examples `DISPLAY:PULSE:STATISTICS:X:SCALE:OFFSET 120` sets the first pulse number to #120.

DISPlay:PULSe:STATistics:Y:RSCale (No Query Form)

Rescales the vertical axis to fit the waveform to the screen in the statistics graph.

Conditions Measurement views: Pulse statistics

Group Display commands

Syntax `DISPlay:PULSe:STATistics:Y:RSCale`

Arguments None

Examples `DISPLAY:PULSE:STATISTICS:Y:RSCALE` rescales the vertical axis of the statistics graph.

DISPlay:PULSe:STATistics:Y[:SCALE]:FULL

Sets or queries the vertical full scale in the statistics graph.

Conditions Measurement views: Pulse statistics

Group Display commands

Syntax `DISPlay:PULSe:STATistics:Y[:SCALE]:FULL <value>`
`DISPlay:PULSe:STATistics:Y[:SCALE]:FULL?`

Related Commands [DISPlay:PULSe:STATistics:X\[:SCALE\]:OFFSet](#)

Arguments `<value>::=<Nrf>` specifies the vertical full scale. The setting range depends on the [DISPlay:PULSe:STATistics:PLOT](#) command parameters and the measurement items as shown in the following table.

DISPlay:PULSe:STATistics:PLOT	Measurement item	Setting range
TRENd	Average on power, Peak power, Average transmitted power	0.1 to 200 dB
	Pulse width, Rise time, Fall time, Repetition interval	1 n to 5 Ms
	Repetition rate	100 m to 100 MHz
	Duty factor, Ripple	1 to 100%
	Droop	1 to 200%
	Pulse-pulse carrier phase	1 to 360°
	FFT	All

Examples `DISPlay:PULSe:STATistics:Y:SCALE:FULL 100` sets the vertical full scale to 100 dB.

DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet

Sets or queries the vertical offset in the statistics graph.

Conditions Measurement views: Pulse statistics

Group Display commands

Syntax `DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet <value>`
`DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet?`

Arguments `<value>::=<NRF>` specifies the vertical offset. The vertical offset is the value at the top or the bottom edge of the graph depending on measurement items. The setting range depends on the [DISPlay:PULSe:STATistics:PLOT](#) command parameters and the measurement items as shown in the table below.

DISPlay:PULSe:STATistics:PLOT	Measurement item	Setting range	Offset position ¹
TRENd	Average on power, Peak power, Average transmitted power	-170 to +50 dBm	Top (Bottom for the unit of Volts or Watts)
	Pulse width, Rise time, Fall time, Repetition interval	0 to 5 Ms	Bottom
	Repetition rate	0 to 100 MHz	Bottom

DISPlay:PULSe :STATistics:PLOT	Measurement item	Setting range	Offset position ¹
	Duty factor, Ripple	0 to 100%	Bottom
	Droop	0 to +100%	Bottom
	Pulse-pulse carrier phase	-180 to +180°	Bottom
FFT	All	-400 to +100 dB	Top

¹ indicates whether the offset is the value at the top or the bottom edge of the graph.

Examples `DISPlay:PULSe:STATISTICS:Y:SCALE:OFFSET 24.8` sets the maximum vertical value to 24.8 dBm in the statistics graph.

DISPlay:PULSe:STATistics:Y[:SCALE]:STOP? (Query Only)

Queries the minimum vertical value (bottom edge) in the statistics graph.

Conditions Measurement views: Pulse statistics

Group Display commands

Syntax `DISPlay:PULSe:STATistics:Y[:SCALE]:STOP?`

Related Commands [DISPlay:PULSe:STATistics:X\[:SCALE\]:OFFSet](#)

Arguments None

Returns `<y_stop>::=<NRF>` is the minimum vertical value (bottom edge).

Examples `DISPlay:PULSe:STATISTICS:Y:SCALE:STOP?` might return `-150.0`, indicating that the minimum vertical value is -150 dBm in the pulse statistics graph.

DISPlay:PULSe:TRACe:MARKer:SHOW:STATE

Determines whether to show or hide the marker readout in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPlay:PULSe:TRACe:MARKer:SHOW:STATE { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:TRACe:MARKer:SHOW:STATE?`

Arguments OFF or 0 hides the marker readout.
 ON or 1 shows the marker readout.

Examples `DISPLAY:PULSE:TRACE:MARKER:SHOW:STATE ON` shows the marker readout on the pulse trace view.

DISP`lay`:PULSe:TRACe:POINT:SHOW

Determines whether to show or hide the measurement points and lines in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPlay:PULSe:TRACe:POINT:SHOW { OFF | ON | 0 | 1 }`
`DISPlay:PULSe:TRACe:POINT:SHOW?`

Arguments OFF or 0 hides the measurement points and lines.
 ON or 1 shows the measurement points and lines.

Examples `DISPLAY:PULSE:TRACE:POINT:SHOW ON` shows the measurement points and lines in the pulse trace view.

DISP`lay`:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATE

Determines whether to show or hide the graticule grid in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATE { OFF
| ON | 0 | 1 }
DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATE?`

Arguments OFF or 0 hides the graticule grid.
ON or 1 shows the graticule grid.

Examples `DISPLAY:PULSE:TRACE:WINDOW:TRACE:GRATICULE:GRID:STATE ON`
shows the graticule grid on the pulse trace view.

DISPPlay:PULSe:TRACe:X:RSCale (No Query Form)

Rescales the horizontal axis to fit the waveform to the screen in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPPlay:PULSe:TRACe:X:RSCale`

Arguments None

Examples `DISPLAY:PULSE:TRACE:X:RSCALE` rescales the horizontal axis in the pulse trace view.

DISPPlay:PULSe:TRACe:X[:SCALE]

Sets or queries the horizontal full scale in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPPlay:PULSe:TRACe:X[:SCALE] <value>
DISPPlay:PULSe:TRACe:X[:SCALE]?`

Arguments <value>::=<Nrf> specifies the horizontal full scale.
Range: 10 ns to acquisition memory capacity.

Examples DISPLAY:PULSE:TRACE:X:SCALE 5.5E-6 sets the horizontal scale to 5.5 μ s.

DISPlay:PULSe:TRACe:X[:SCALe]:FULL

Sets or queries the full-scale reference for the horizontal rescale.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax DISPlay:PULSe:TRACe:X[:SCALe]:FULL { SELEcted | MAXimum }
DISPlay:PULSe:TRACe:X[:SCALe]:FULL?

Arguments SELEcted uses the selected pulse for the full-scale reference.
MAXimum uses the maximum pulse for the full-scale reference.

Examples DISPLAY:PULSE:TRACE:X:SCALE:FULL SELEcted uses the selected pulse for the full-scale reference.

DISPlay:PULSe:TRACe:X[:SCALe]:OFFSet

Sets or queries the minimum horizontal value (left edge) in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax DISPlay:PULSe:TRACe:X[:SCALe]:OFFSet <value>
DISPlay:PULSe:TRACe:X[:SCALe]:OFFSet?

Related Commands [DISPlay:PULSe:TRACe:X\[:SCALe\]:PDIVision](#)

Arguments `<value> ::= <NRf>` specifies the minimum horizontal value.
 Range: $[(\text{analysis offset}) - (\text{X scale}) \times 0.9]$ to $[(\text{analysis offset}) + (\text{analysis length}) - (\text{X scale}) \times 0.1]$

Examples `DISPLAY:PULSE:TRACE:X:SCALE:OFFSET 937.5E-9` sets the minimum horizontal value to 937.5 ns.

DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision

Sets or queries the horizontal full scale in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision <value>`
`DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision?`

Arguments `<value> ::= <NRf>` specifies the horizontal full scale.
 Range: 10 ns to acquisition memory capacity.

Examples `DISPLAY:PULSE:TRACE:X:SCALE:PDIVISION 5.5E-6` sets the horizontal scale to 5.5 μ s.

DISPlay:PULSe:TRACe:Y:RSCale (No Query Form)

Rescales the vertical axis to fit the waveform to the screen in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPlay:PULSe:TRACe:Y:RSCale`

Arguments None

Examples `DISPLAY:PULSE:TRACE:Y:RSCALE` rescales the vertical axis in the pulse trace view.

DISPlay:PULSe:TRACe:Y[:SCALe]:FULL

Sets or queries the vertical full scale in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPlay:PULSe:TRACe:Y[:SCALe]:FULL <value>`
`DISPlay:PULSe:TRACe:Y[:SCALe]:FULL?`

Related Commands [DISPlay:PULSe:TRACe:Y\[:SCALe\]:OFFSet](#)

Arguments `<value>::=<Nrf>` specifies the vertical full scale.
 Range: 0.1 to 200 dB.
 The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `DISPLAY:PULSE:TRACE:Y:SCALE:FULL 100` sets the vertical full scale to 100 dB.

DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax `DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet <value>`
`DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet?`

Related Commands [DISPlay:PULSe:TRACe:Y\[:SCALe\]:STOP?](#)

Arguments <value>::=<Nrf> specifies the vertical offset. Range: -170 to +50 dBm.

Examples DISPLAY:PULSE:TRACE:Y:SCALE:OFFSET 23.5 sets the vertical offset to 23.5 dBm.

DISPlay:PULSe:TRACe:Y[:SCALE]:STOP? (Query Only)

Queries the minimum vertical value (bottom edge) in the pulse trace view.

Conditions Measurement views: Pulse trace

Group Display commands

Syntax DISPlay:PULSe:TRACe:Y[:SCALE]:STOP?

Related Commands [DISPlay:PULSe:TRACe:Y\[:SCALE\]:OFFSet](#)

Arguments None

Returns <y_stop>::=<Nrf> is the minimum vertical value (bottom edge).

Examples DISPLAY:PULSE:TRACE:Y:SCALE:STOP? might return -150.0, indicating that the minimum vertical value is -150 dBm in the pulse trace view.

DISPlay:SGRam:FREQuency:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the spectrogram view.

Conditions Measurement views: Spectrogram

Group Display commands

Syntax DISPlay:SGRam:FREQuency:AUTO

Arguments None

Examples `DISPLAY:SGRAM:FREQUENCY:AUTO` rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:SGRam:FREQuency:OFFSet

Sets or queries the frequency offset (the value at the center of the horizontal axis) in the spectrogram.

Conditions Measurement views: Spectrogram

Group Display commands

Syntax `DISPly:SGRam:FREQuency:OFFSet <value>`
`DISPly:SGRam:FREQuency:OFFSet?`

Related Commands [DISPlay:SPECTrum:FREQuency\[:SCALE\]](#)

Arguments `<value>::=<Nrf>` specifies the frequency offset.
 Range: [(center frequency) - (X scale) × 0.9] to [(center frequency) + (X scale) × 0.9]

Examples `DISPLAY:SGRAM:FREQUENCY:OFFSET 1.45GHZ` sets the frequency offset to 1.45 GHz in the spectrogram.

DISPlay:SGRam:FREQuency:SCALE

Sets or queries the horizontal range of the spectrogram.

Conditions Measurement views: Spectrogram

Group Display commands

Syntax `DISPly:SGRam:FREQuency:SCALE <value>`
`DISPly:SGRam:FREQuency:SCALE?`

Related Commands [DISPlay:SPECTrum:FREQuency:OFFSet](#)

Arguments <value> ::= <NRF> specifies the horizontal range.
Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples DISPLAY:SGRAM:FREQUENCY:SCALE 10MHZ sets the horizontal range to 10 MHz.

DISPlay:SGRam:TIME:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the graph to the screen in the spectrogram view.

Conditions Measurement views: Spectrogram

Group Display commands

Syntax DISPlay:SGRam:TIME:AUTO

Arguments None

Examples DISPLAY:SGRAM:TIME:AUTO rescales the vertical scale automatically to fit the waveform to the screen.

DISPlay:SGRam:TIME:OFFSet

Sets or queries the vertical axis (time) offset (bottom line number) in the spectrogram.

Conditions Measurement views: Spectrogram

Group Display commands

Syntax DISPlay:SGRam:TIME:OFFSet <value>
DISPlay:SGRam:TIME:OFFSet?

Related Commands [DISPlay:SGRam:TIME:SCAle](#)

Arguments <value>::=<Nrf> specifies the time offset.
Range: Line #0 to 125000. Zero (0) represents the latest line.

Examples DISPLAY:SGRAM:TIME:OFFSET 15 sets the time offset to Line #15.

DISPlay:SGRam:TIME:OVERlap

Determines whether or not to allow overlap between adjacent FFT frames on the time axis in the spectrogram.

Conditions Measurement views: Spectrogram

Group Display commands

Syntax DISPlay:SGRam:TIME:OVERlap { OFF | ON | 0 | 1 }
DISPlay:SGRam:TIME:OVERlap?

Arguments OFF or 0 inhibits overlap between adjacent FFT frames on the time axis.
ON or 1 allows overlap between adjacent FFT frames on the time axis.

Examples DISPLAY:SGRAM:TIME:OVERLAP ON allows overlap between adjacent FFT frames on the time axis in the spectrogram.

DISPlay:SGRam:TIME:SCALE

Sets or queries the vertical scale (the amount of time in each line) in the spectrogram. The vertical axis is composed of successive spectral displays. The new spectra can be added at a timed rate specified by this command. For example, if you set the scale to -5, one line is displayed every 5 spectra.

Conditions Measurement views: Spectrogram

Group Display commands

Syntax DISPlay:SGRam:TIME:SCALE <value>
DISPlay:SGRam:TIME:SCALE?

Related Commands [DISPlay:SGRam:TIME:OFFSet](#)

Arguments <value>::=<NR1> specifies the vertical scale.
Range: -1023 to 0. Zero (0) displays every spectrum.

Examples DISPLAY:SGRAM:TIME:SCALE -5 displays one line every 5 spectra in the spectrogram.

DISPlay:SPECTrum:FREQuency:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the spectrum view.

Conditions Measurement views: Spectrum

Group Display commands

Syntax DISPlay:SPECTrum:FREQuency:AUTO

Arguments None

Examples DISPLAY:SPECTRUM:FREQUENCY:AUTO rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:SPECTrum:FREQuency:OFFSet

Sets or queries the frequency offset (the value at the center of the horizontal axis) in the spectrum graph.

Conditions Measurement views: Spectrum

Group Display commands

Syntax DISPlay:SPECTrum:FREQuency:OFFSet <value>
DISPlay:SPECTrum:FREQuency:OFFSet?

Related Commands [DISPlay:SPECTrum:FREQuency\[:SCALE\]](#)

Arguments <value>::=<Nrf> specifies the frequency offset.
 Range: [(center frequency) - (X scale) × 0.9] to [(center frequency) + (X scale) × 0.9]

Examples DISPLAY:SPECTRUM:FREQUENCY:OFFSET 1.45GHZ sets the frequency offset to 1.45 GHz in the spectrum.

DISPlay:SPECTrum:FREQuency[:SCAlE]

Sets or queries the horizontal range of the spectrum graph.

Conditions Measurement views: Spectrum

Group Display commands

Syntax DISPlay:SPECTrum:FREQuency[:SCAlE] <value>
 DISPlay:SPECTrum:FREQuency[:SCAlE]?

Related Commands [DISPlay:SPECTrum:FREQuency:OFFSet](#)

Arguments <value>::=<Nrf> specifies the horizontal range.
 Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples DISPLAY:SPECTRUM:FREQUENCY:SCALE 10MHZ sets the horizontal range to 10 MHz.

DISPlay:SPECTrum:MARKer:NOISe:MODE

Determines whether to enable or disable the marker noise mode in the spectrum view. In this mode, the marker readout indicates amplitude in dBm/Hz. It is valid for all markers except for the reference marker.

NOTE. To use the marker noise mode, select dBm as the power unit by the [SENSe]:POWer:UNITs command.

Conditions Measurement views: Spectrum

Group Display commands

Syntax `DISPlay:SPECTrum:MARKer:NOISE:MODE { OFF | ON | 0 | 1 }`
`DISPlay:SPECTrum:MARKer:NOISE:MODE?`

Related Commands [\[SENSE\]:POWER:UNITS](#)

Arguments OFF or 0 disables the marker noise mode.
ON or 1 enables the marker noise mode.

Examples `DISPLAY:SPECTRUM:MARKER:NOISE:MODE ON` enables the marker noise mode.

DISPlay:SPECTrum:SCALE:LOG:STATE

Determines whether or not to set the horizontal axis logarithmic in the Spectrum view.

Conditions Measurement views: Spectrum

Group Display commands

Syntax `DISPlay:SPECTrum:SCALE:LOG:STATE { OFF | ON | 0 | 1 }`
`DISPlay:SPECTrum:SCALE:LOG:STATE?`

Related Commands [DISPlay:SPECTrum:X:LABEL](#)

Arguments OFF or 0 sets the horizontal axis linear (default).
ON or 1 sets the horizontal axis logarithmic.
Executing `DISPlay:SPECTrum:SCALE:LOG:STATE ON` sets
`DISPlay:SPECTrum:X:LABEL SSFReq`.

Examples `DISPLAY:SPECTRUM:SCALE:LOG:STATE ON` sets the horizontal axis
logarithmic in the Spectrum view.

DISPlay:SPECTrum:WINDow:TRACe:GRATICule:GRID:STATE

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: Spectrum

Group	Display commands
Syntax	DISP <code>l</code> ay:SPECT <code>r</code> um:WIND <code>o</code> w:TRAC <code>e</code> :GRATIC <code>u</code> le:GRID:STATE { OFF ON 0 1 } DISP <code>l</code> ay:SPECT <code>r</code> um:WIND <code>o</code> w:TRAC <code>e</code> :GRATIC <code>u</code> le:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISP <code>l</code> AY:SPECT <code>R</code> UM:WIND <code>O</code> W:TRAC <code>E</code> :GRATIC <code>U</code> LE:GRID:STATE ON shows the graticule grid on the screen in the spectrum measurement.

DISP`l`ay:SPECT`r`um:WIND`o`w:TRAC`e`:LEG`e`nd:STAT`e`

Determines whether to show or hide the trace legend in the Spectrum view. The legend indicates the trace detection and function on the screen for each displayed spectrum trace.

Conditions	Measurement views: Spectrum
Group	Display commands
Syntax	DISP <code>l</code> ay:SPECT <code>r</code> um:WIND <code>o</code> w:TRAC <code>e</code> :LEG <code>e</code> nd:STATE { OFF ON 0 1 } DISP <code>l</code> ay:SPECT <code>r</code> um:WIND <code>o</code> w:TRAC <code>e</code> :LEG <code>e</code> nd:STATE?
Arguments	OFF or 0 hides the trace legend. ON or 1 shows the trace legend.
Examples	DISP <code>l</code> AY:SPECT <code>R</code> UM:WIND <code>O</code> W:TRAC <code>E</code> :LEG <code>E</code> ND:STATE ON shows the trace legend on the screen in the spectrum measurement.

DISP`l`ay:SPECT`r`um:X:LAB`e`l

Sets or queries the labels for the horizontal (X) axis in the Spectrum view. The labels are indicated beneath the spectrum graph on the screen.

Conditions	Measurement views: Spectrum
-------------------	-----------------------------

Group	Display commands
Syntax	DISPlay:SPECTrum:X:LABE1 { SSFReq CFSPan } DISPlay:SPECTrum:X:LABE1?
Arguments	SSFReq sets the labels to the start and stop frequencies. CFSPan sets the labels to the center frequency and span.
Examples	DISPLAY:SPECTRUM:X:LABEL SSFReq sets the labels to the start and stop frequencies for the horizontal axis in the Spectrum view.

DISPlay:SPECTrum:Y[:SCALE]

Sets or queries the vertical range of the spectrum graph.

Conditions	Measurement views: Spectrum
Group	Display commands
Syntax	DISPlay:SPECTrum:Y[:SCALE] <value> DISPlay:SPECTrum:Y[:SCALE]?
Arguments	<value> ::= <NRf> specifies the vertical range. Range: 0.1 to 200 dB. The amplitude unit is set by the [SENSe]:POWer:UNITs command. You can omit the unit in the argument. When you include the unit in the argument, only dB is available. For the amplitude units Watts, Volts, and Amps, omit the unit in the argument.
Examples	DISPLAY:SPECTRUM:Y:SCALE 50dB sets the vertical range to 50 dB in the Spectrum view.

DISPlay:SPECTrum:Y[:SCALE]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Spectrum view.

Conditions	Measurement views: Spectrum
-------------------	-----------------------------

Group	Display commands
Syntax	DISP <code>lay</code> :SPECT <code>rum</code> :Y[:SCALE]:AUTO
Arguments	None
Examples	DISP <code>lay</code> :SPECT <code>rum</code> :Y:SCALE:AUTO rescales the vertical scale automatically to fit the waveform to the screen.

DISP`lay`:SPECT`rum`:Y[:SCALE]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) of the spectrum graph.

Conditions	Measurement views: Spectrum
Group	Display commands
Syntax	DISP <code>lay</code> :SPECT <code>rum</code> :Y[:SCALE]:OFFSet <value> DISP <code>lay</code> :SPECT <code>rum</code> :Y[:SCALE]:OFFSet?
Arguments	<value>::=<NRF> specifies the vertical offset. Range: -270 to +150 dBm. The amplitude unit is set by the [SENSE]:POWER:UNITS command (default: dBm). You can omit the unit in the argument. When you include the unit in the argument, only dBm is allowed. For the other amplitude units, omit the unit in the argument.
Examples	DISP <code>lay</code> :SPECT <code>rum</code> :Y:SCALE:OFFSet -12.5dBm sets the vertical offset to -12.5 dBm.

DISP`lay`:SPECT`rum`:Y[:SCALE]:PDIVision

Sets or queries the vertical scale (per division) of the spectrum graph.

Conditions	Measurement views: Spectrum
Group	Display commands

Syntax `DISPlay:SPECTrum:Y[:SCALE]:PDIVision <value>`
`DISPlay:SPECTrum:Y[:SCALE]:PDIVision?`

Related Commands [\[SENSe\]:POWer:UNITs](#)

Arguments `<value> ::= <NRF>` specifies the vertical scale (per division).
Range: 0.01 to 20 dB/div.

Examples `SENSE:SPECTRUM:Y:SCALE:PDIVISION 0.5` sets the vertical scale to 0.5 dB/div.

DISPlay:SPECTrum:Y[:SCALE]:RESet (No Query Form)

Resets the vertical scale of the spectrum graph to the default values:
Vertical offset = Reference level and Vertical scale = 100 dB

Conditions Measurement views: Spectrum

Group Display commands

Syntax `DISPlay:SPECTrum:Y[:SCALE]:RESet`

Arguments None

Examples `DISPLAY:SPECTRUM:Y:SCALE:RESET` resets the vertical scale to the default values in the Spectrum view.

DISPlay:SPURious:MARKer:SHOW:STATe

Determines whether to show or hide the readout for the selected marker in the Spurious view.

Conditions Measurement views: Spurious

Group Display commands

Syntax `DISPlay:SPURious:MARKer:SHOW:STATE { OFF | ON | 0 | 1 }`
`DISPlay:SPURious:MARKer:SHOW:STATE?`

Arguments OFF or 0 hides the readout for the selected marker in the graph.
 ON or 1 shows the readout for the selected marker in the graph.

Examples `DISPLAY:SPURIOUS:MARKER:SHOW:STATE ON` shows the readout for the selected marker in the graph.

DISPlay:SPURious:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the Spurious view.

Vertical offset = 0 dBm,
 Vertical scale = 100 dB,
 Horizontal offset = Center frequency, and
 Horizontal scale = Default span

Conditions Measurement views: Spurious

Group Display commands

Syntax `DISPlay:SPURious:RESet:SCALE`

Arguments None

Examples `DISPLAY:SPURIOUS:RESET:SCALE` resets the horizontal and vertical scale to the default values.

DISPlay:SPURious:SCALE:LOG:STATE

Determines whether or not to set the horizontal axis logarithmic in the Spurious view.

Conditions Measurement views: Spurious

Group Display commands

Syntax	<code>DISPlay:SPURious:SCALE:LOG:STATe { OFF ON 0 1 }</code> <code>DISPlay:SPURious:SCALE:LOG:STATe?</code>
Arguments	OFF or 0 sets the horizontal axis linear (default). ON or 1 sets the horizontal axis logarithmic.
Examples	<code>DISPLAY:SPURIOUS:SCALE:LOG:STATE ON</code> sets the horizontal axis logarithmic in the Spurious view.

DISPlay:SPURious:SElect:NUMBer

Sets or queries the spurious number in the Spurious view.

Conditions	Measurement views: Spurious
Group	Display commands
Syntax	<code>DISPlay:SPURious:SElect:NUMBer <number></code> <code>DISPlay:SPURious:SElect:NUMBer?</code>
Arguments	<code><number>::=<NR1></code> specifies the spurious number. Range: 1 to the number of spurious signals. Use the FETCh:SPURious:COUNT? or READ:SPURious:COUNT? query to get the number of spurious signals.
Examples	<code>DISPLAY:SPURIOUS:SELECT:NUMBER 7</code> selects the spurious #7.

DISPlay:SPURious:SHOW:LIMit

Sets or queries how to display the limits.

Conditions	Measurement views: Spurious
Group	Display commands
Syntax	<code>DISPlay:SPURious:SHOW:LIMit { SHADEd LINE OFF }</code> <code>DISPlay:SPURious:SHOW:LIMit?</code>

Arguments	<p>SHADed displays the limits with shade.</p> <p>LINE displays the limits with line only.</p> <p>OFF hides the limits.</p>
Examples	<p>DISPLAY:SPURIOUS:SHOW:LIMIT LINE displays the limits with line only.</p>

DISPlay:SPURious:WINDow:TRACe:GRATICule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Spurious
Group	Display commands
Syntax	<p>DISP<code>l</code>ay:SPUR<code>i</code>ous:WIND<code>o</code>w:TRAC<code>e</code>:GRATIC<code>u</code>le:GRID:STAT<code>e</code> { OFF ON 0 1 }</p> <p>DISP<code>l</code>ay:SPUR<code>i</code>ous:WIND<code>o</code>w:TRAC<code>e</code>:GRATIC<code>u</code>le:GRID:STAT<code>e</code>?</p>
Arguments	<p>OFF or 0 hides the graticule grid.</p> <p>ON or 1 shows the graticule grid.</p>
Examples	<p>DISPLAY:SPURIOUS:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen.</p>

DISPlay:SPURious:X[:SCALe]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the Spurious view.

Conditions	Measurement views: Spurious
Group	Display commands
Syntax	<p>DISP<code>l</code>ay:SPUR<code>i</code>ous:X[:SCAL<code>e</code>]:AUTO</p>
Arguments	None

Examples `DISPLAY:SPURIOUS:X:SCALE:AUTO` rescales the horizontal scale automatically to fit the waveform to the screen.

DISPlay:SPURious:X[:SCALe]:START

Sets or queries the minimum horizontal value (left edge) of the spectrum graph in the Spurious view.

Conditions Measurement views: Spurious

Group Display commands

Syntax `DISPlay:SPURious:X[:SCALe]:START <value>`
`DISPlay:SPURious:X[:SCALe]:START?`

Arguments `<value> ::= <NRF>` specifies the minimum horizontal value.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples `DISPLAY:SPURIOUS:X:SCALE:START 1.61GHZ` sets the minimum horizontal value to 1.61 GHz in the spectrum graph.

DISPlay:SPURious:X[:SCALe]:STOP

Sets or queries the maximum horizontal value (right edge) of the spectrum graph in the Spurious view.

Conditions Measurement views: Spurious

Group Display commands

Syntax `DISPlay:SPURious:X[:SCALe]:STOP <value>`
`DISPlay:SPURious:X[:SCALe]:STOP?`

Arguments `<value> ::= <NRF>` specifies the minimum horizontal value.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples `DISPLAY:SPURIOUS:X:SCALE:STOP 2.16GHZ` sets the maximum horizontal value to 2.16 GHz in the spectrum graph.

DISPlay:SPURious:Y[:SCALe]

Sets or queries the vertical range of the spectrum graph in the Spurious view.

Conditions	Measurement views: Spurious
Group	Display commands
Syntax	DISPlay:SPURious:Y[:SCALe] <value> DISPlay:SPURious:Y[:SCALe]?
Arguments	<value>::=<NRF> specifies the vertical range. Range: 0.1 to 200 dB. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	DISPlay:SPURious:Y:SCALE 100 sets the vertical range to 100 dB in the Spurious view.

DISPlay:SPURious:Y[:SCALe]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Spurious view.

Conditions	Measurement views: Spurious
Group	Display commands
Syntax	DISPlay:SPURious:Y[:SCALe]:AUTO
Arguments	None
Examples	DISPlay:SPURious:Y:SCALE:AUTO rescales the vertical scale automatically to fit the waveform to the screen.

DISPlay:SPURious:Y[:SCALe]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) of the spectrum graph in the Spurious view.

Conditions	Measurement views: Spurious
Group	Display commands
Syntax	DISPlay:SPURious:Y[:SCALE]:OFFSet <value> DISPlay:SPURious:Y[:SCALE]:OFFSet?
Arguments	<value> ::= <NRF> specifies the vertical offset. Range: -270 to +150 dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	DISPlay:SPURIOUS:Y:SCALE:OFFSET -12.5 sets the vertical offset to -12.5 dBm in the spectrum graph.

DISPlay:TDIagram:WINDow:TRACe:GRATICule:GRID:STATE

Determines whether to show or hide the graticule grid on the screen.

Conditions	Measurement views: Trellis diagram
Group	Display commands
Syntax	DISPlay:TDIagram:WINDow:TRACe:GRATICule:GRID:STATE { OFF ON 0 1 } DISPlay:TDIagram:WINDow:TRACe:GRATICule:GRID:STATE?
Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
Examples	DISPlay:TDIAGRAM:WINDOW:TRACE:GRATICULE:GRID:STATE ON shows the graticule grid on the screen in the trellis diagram.

DISPlay:TDIagram:Y[:SCALE]

Sets or queries the vertical range of the trellis diagram.

Conditions	Measurement views: Trellis diagram
-------------------	------------------------------------

Group	Display commands
Syntax	DISP <code>lay:TDIagram:Y[:SCALE]</code> <value> DISP <code>lay:TDIagram:Y[:SCALE]</code> ?
Arguments	<value>::=<NRF> specifies the vertical range. Range: 1 ° to 1 T°.
Examples	DISP <code>lay:TDIAGRAM:Y:SCALE</code> 2.5 sets the vertical range to 2.5 ° in the trellis diagram.

DISP`lay:TDIagram:Y[:SCALE]:AUTO` (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the trellis diagram.

Conditions	Measurement views: Trellis diagram
Group	Display commands
Syntax	DISP <code>lay:TDIagram:Y[:SCALE]:AUTO</code>
Arguments	None
Examples	DISP <code>lay:TDIAGRAM:Y:SCALE:AUTO</code> sets the vertical scale automatically to fit the waveform to the screen.

DISP`lay:TDIagram:Y[:SCALE]:OFFSet`

Sets or queries the vertical offset (center point of the vertical axis) of the Trellis diagram.

Conditions	Measurement views: Trellis diagram
Group	Display commands
Syntax	DISP <code>lay:TDIagram:Y[:SCALE]:OFFSet</code> <value> DISP <code>lay:TDIagram:Y[:SCALE]:OFFSet</code> ?

Arguments <value> ::= <Nrf> specifies the vertical offset. Range: -1 T° to +1 T°.

Examples DISPLAY:TDIAGRAM:Y:SCALE:OFFSET -28.5 sets the vertical offset to -28.5 ° in the Trellis diagram.

DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe

Determines whether to show or hide the graticule grid on the screen.

Conditions Measurement views: Time overview

Group Display commands

Syntax DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe { OFF | ON | 0 | 1 }
DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
ON or 1 shows the graticule grid.

Examples DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe ON shows the graticule grid on the screen in the time overview.

DISPlay:TOVerview:X[:SCALE]

Sets or queries the horizontal scale (full-scale time) of the time overview.

Conditions Measurement views: Time overview

Group Display commands

Syntax DISPlay:TOVerview:X[:SCALE] <value>
DISPlay:TOVerview:X[:SCALE]?

Related Commands [DISPlay:TOVerview:X\[:SCALE\]:OFFSet](#)

Arguments <value>::=<Nrf> specifies the horizontal scale in full-scale time.
 Range: 10 ns to the acquisition memory capacity.
 You can see the acquisition memory capacity using the [\[SENSe\]:ACquisition:MEMory:CAPacity\[:TIME\]?](#) query.

Examples DISPLAY:TOVERVIEW:X:SCALE 12.5us sets the horizontal scale to 12.5 μ s.

DISPlay:TOVerview:X[:SCALE]:AUTO (No Query Form)

Sets the horizontal scale and offset automatically to fit the waveform to the screen in the time overview.

Conditions Measurement views: Time overview

Group Display commands

Syntax DISPlay:TOVerview:X[:SCALE]:AUTO

Arguments None

Examples DISPLAY:TOVERVIEW:X:SCALE:AUTO sets the horizontal scale and offset automatically to fit the waveform to the screen.

DISPlay:TOVerview:X[:SCALE]:OFFSet

Sets or queries the minimum horizontal value (left edge) of the time overview.

Conditions Measurement views: Time overview

Group Display commands

Syntax DISPlay:TOVerview:X[:SCALE]:OFFSet <value>
 DISPlay:TOVerview:X[:SCALE]:OFFSet?

Related Commands [DISPlay:TOVerview:X\[:SCALE\]](#)

Arguments `<value> ::= <NRf>` specifies the minimum horizontal value.
 Range: $[(\text{analysis offset}) - (\text{X scale}) \times 0.9]$ to $[(\text{analysis offset}) + (\text{analysis length}) - (\text{X scale}) \times 0.1]$

Examples `DISPLAY:TOVERVIEW:X:SCALE:OFFSET 800ns` sets the minimum horizontal value to 800 ns in the time overview.

DISPlay:TOVerview:Y[:SCALE]

Sets or queries the vertical range of the time overview.

Conditions Measurement views: Time overview

Group Display commands

Syntax `DISPlay:TOVerview:Y[:SCALE] <value>`
`DISPlay:TOVerview:Y[:SCALE]?`

Related Commands [DISPlay:TOVerview:Y\[:SCALE\]:OFFSet](#)

Arguments `<value> ::= <NRf>` specifies the vertical range. Range: 0.1 to 200 dB.

Examples `DISPLAY:TOVERVIEW:Y:SCALE 50` sets the vertical range to 50 dBm in the time overview.

DISPlay:TOVerview:Y[:SCALE]:AUTO (No Query Form)

Sets the vertical scale and offset automatically to fit the waveform to the screen in the time overview.

Conditions Measurement views: Time overview

Group Display commands

Syntax `DISPlay:TOVerview:Y[:SCALE]:AUTO`

Arguments None

Examples `DISPLAY:TOVERVIEW:Y:SCALE:AUTO` sets the vertical scale and offset automatically to fit the waveform to the screen.

DISPlay:TOVerview:Y[:SCALe]:OFFSet

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the time overview.

Conditions Measurement views: Time overview

Group Display commands

Syntax `DISPlay:TOVerview:Y[:SCALe]:OFFSet <value>`
`DISPlay:TOVerview:Y[:SCALe]:OFFSet?`

Related Commands [DISPlay:TOVerview:Y\[:SCALe\]](#)

Arguments `<value>::=<NRF>` specifies the vertical offset. Range: -170 to +50 dBm.

Examples `DISPLAY:TOVERVIEW:Y:SCALE:OFFSET -80` sets the vertical offset to -80 dBm in the time overview.

DISPlay:TOVerview:Y[:SCALe]:RESCale (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the time overview.

Conditions Measurement views: Time overview

Group Display commands

Syntax `DISPlay:TOVerview:Y[:SCALe]:RESCale`

Arguments None

Examples `DISPLAY:TOVERVIEW:Y:SCALE:RESCALE` sets the vertical scale automatically to fit the waveform to the screen.

DISPlay:WINDow:ACTive:MEASurement? (Query Only)

Queries the active measurement views.

Conditions	Measurement views: All
Group	Display commands
Syntax	DISPlay:WINDow:ACTive:MEASurement?
Arguments	None
Returns	<view1>,<view2>,...,<view(n)>

Where

<view(n)> ::= <string> is the view name as shown in the following table.

Table 2-33: Measurement view mnemonic

Return value	Measurement view	Display group
"SPEC	Spectrum	General signal viewing
"DPSA"	DPX (Digital Phosphor) spectrum	
"MAGVT"	Amplitude versus Time	
"ACP"	Channel power and ACPR	
"FVT"	Frequency versus Time	
"PHVT"	Phase versus Time	
"IQVT"	RF I&Q versus Time	
"SGRam"	Spectrogram	
"TOV"	Time overview	
"AM"	Amplitude modulation	
"FM"	Frequency modulation	
"PM"	Phase modulation	

Table 2-33: Measurement view mnemonic (cont.)

Return value	Measurement view	Display group
"CONS"	Constellation	General purpose digital modulation
"DIQV"	Demodulated I&Q versus Time	
"EDI"	Eye Diagram	
"EVM"	EVM versus Time	
"FVDT"	Frequency deviation versus Time	
"MERR"	Magnitude error versus Time	
"PERR"	Phase error versus Time	
"SIGN"	Signal quality	
"STAB"	Symbol table	
"TDI"	Trellis Diagram	
"CCDF"	CCDF	RF measurements
"MCP"	MCPR (Multiple Carrier Power Ratio)	
"OBW"	Occupied bandwidth	
"PNO"	Phase noise	
"SPUR"	Spurious	
"STAT"	Pulse statistics	Pulsed RF
"RES"	Pulse table (results table)	
"TRAC"	Pulse trace	

Examples `DISPLAY:WINDOW:ACTIVE:MEASUREMENT?` might return "SPEC", "TRAC", indicating that the views of spectrum and pulse trace are displayed on the screen.

DISPlay:WINDow:COLor:SCHEME

Sets or queries the color scheme for displaying traces and background on the screen.

Conditions Measurement views: All

Group Display commands

Syntax `DISPlay:WINDow:COLor:SCHEME { THUNDERstorm | BLIZZard | CLASSic }`
`DISPlay:WINDow:COLor:SCHEME?`

Arguments	<p>THUNDERstorm displays the background in dark blue.</p> <p>BLIZZard displays the background in white. It saves ink when printing the screen image.</p> <p>CLASSic displays the background in black (default).</p>
Examples	DISPLAY:WINDOW:COLOR:SCHEME BLIZZard displays the background in white.

DISPlay:WINDow:OPTimized:MEASurement? (Query Only)

Queries the measurement views that are optimized. "Optimized" means that there is a perfect match between the view's settings and the actual acquisition parameters to meet the specifications. When multiple measurements are running at one time, the measurements can have different requirements for setting the acquisition hardware. You can make a measurement optimized by selecting it using the following commands:

- [DISPlay:GENeral:MEASview:SElect](#) for the general signal viewing
- [DISPlay:DDEMod:MEASview:SElect](#) for the digital modulation views
- [DISPlay:GPRF:MEASview:SElect](#) for the RF measurement views
- [DISPlay:PULSe:MEASview:SElect](#) for the pulsed RF measurement views

Conditions	Measurement views: All
Group	Display commands
Syntax	DISPlay:WINDow:OPTimized:MEASurement?
Arguments	None
Returns	<p><view1>,<view2>,...,<view(n)></p> <p>Where <view(n)>::=<string> is the view name as shown in the table. (See Table 2-33 on page 2-355.)</p>
Examples	DISPLAY:WINDOW:OPTIMIZED:MEASUREMENT? might return "SPEC", "MCP", indicating that the views of spectrum and MCPR are optimized.

*ESE

Sets or queries the bits in the Event Status Enable Register (ESER). The ESER prevents events from being reported to the Status Byte Register (STB). Refer to Section 3, *Status and Events*, for the register information.

Conditions	Measurement views: All
Group	IEEE common commands
Syntax	*ESE <value> *ESE?
Related Commands	*CLS , *ESR? , *SRE , *STB?
Arguments	<value> ::= <NR1> is a value in the range from 0 through 255. The binary bits of the ESER are set according to this value.
Examples	*ESE 145 sets the ESER to binary 10010001, which enables the PON, EXE, and OPC bits. *ESE? might return the string *ESE 184, showing that the ESER contains the binary value 10111000.

*ESR? (Query Only)

Returns the contents of the Standard Event Status Register (SESR). *ESR? also clears the SESR (since reading the SESR clears it). Refer to Section 3, *Status and Events*, for the register information.

Conditions	Measurement views: All
Group	IEEE common commands
Syntax	*ESR?
Related Commands	*CLS , *ESE , *SRE , *STB?
Arguments	None

Returns <NR1> representing the contents of the SESR by a 0 to 255 decimal number.

Examples *ESR? might return the value 213, showing that the SESR contains binary 11010101.

FETCh:ACPower? (Query Only)

Returns the Channel power and ACPR measurement results for all available channels.

Conditions Measurement views: Channel power and ACPR

Group Fetch commands

Syntax FETCh:ACPower?

Arguments None

Returns <chan_power>, <acpr_lower(1)>, <acpr_upper(1)>, <acpr_lower(2)>, <acpr_upper(2)>, . . . <acpr_lower(n)>, <acpr_upper(n)>

Where

<chan_power> is the average power of the main channel as the power reference in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.

<acpr_lower(n)> is the ACPR for the lower channel #n in dB.

<acpr_upper(n)> is the ACPR for the upper channel #n in dB.

The number of n depends on the setting of the [SENSe]:ACPower:CHANnel:PAIRs command.

Examples FETCh:ACPOWER? might return 4.227, -28.420, -23.847, -22.316, -29.225, indicating (average power of the main channel) = 4.227 dBm, (ACPR for the lower channel 1) = -28.420 dB, (ACPR for the upper channel 1) = -23.847 dB, (ACPR for the lower channel 2) = -22.316 dB, and (ACPR for the upper channel 2) = -29.225 dB.

FETCh:ACPower:CHANnel:POWer? (Query Only)

Returns the average power of the main channel (power reference) in the Channel power and ACPR measurement.

Conditions	Measurement views: Channel power and ACPR
Group	Fetch commands
Syntax	FETCh:ACPower:CHANnel:POWer?
Arguments	None
Returns	<chan_power> ::= <Nrf> is the average power of the main channel in dBm. The unit can be changed by the [SENSE]:POWER:UNITs command.
Examples	FETCh:ACPower:CHANnel:POWer? might return 4.227, indicating that the average power of the main channel is 4.227 dBm.

FETCh:ACPower:SPECTrum? (Query Only)

Returns spectrum trace data of the Channel power and ACPR measurement.

Conditions	Measurement views: Channel power and ACPR
Group	Fetch commands
Syntax	FETCh:ACPower:SPECTrum?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude in dBm at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `FETCH:ACPOWER:SPECTRUM?` might return `#43204xxxx...` (3204-byte data) for the spectrum trace data of the Channel power and ACPR measurement.

FETCH:{AM|FM|PM}? (Query Only)

Returns the trace data in the AM/FM/PM measurement.

Conditions Measurement views: AM, FM, and PM

Group Fetch commands

Syntax `FETCH:{AM|FM|PM}?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the modulation factor in percent (AM), frequency deviation in Hz (FM), or phase deviation in degrees (PM) at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:AM?` might return `#3156xxxx...` (156-byte data) for the AM measurement trace.

FETCH:AM:AMINdex? (Query Only)

Returns the modulation depth which is the (positive peak modulation factor - negative peak modulation factor)/2 returned as a percentage (%).

Conditions Measurement views: AM

Group Fetch commands

Syntax FETCh:AM:AMINdex?

Arguments None

Returns <value>::=<NRF> the modulation index.

Examples FETCh:AM:AMINDEX? might return 77.1854035556E-3 , indicating the modulation index is 0.0772% or 77.2 m%.

FETCh:AM:AMNegative? (Query Only)

Returns the negative peak modulation factor (–AM) in the AM measurement.

Conditions Measurement views: AM

Group Fetch commands

Syntax FETCh:AM:AMNegative?

Arguments None

Returns <-AM>::=<NRF> is the negative peak modulation factor in percent (%).

Examples FETCh:AM:AMNEGATIVE? might return –23.4, indicating the negative peak modulation factor is –23.4%.

FETCh:AM:AMPositive? (Query Only)

Returns the positive peak modulation factor (+AM) in the AM measurement.

Conditions Measurement views: AM

Group Fetch commands

Syntax FETCh:AM:AMPositive?

Arguments	None
Returns	<+AM> ::= <NRf> is the positive peak modulation factor in percent (%).
Examples	FETCH:AM:AMPOSITIVE? might return 43.8, indicating the positive peak modulation factor is 43.8%.

FETCH:AM:RESult? (Query Only)

Returns the AM measurement results.

Conditions	Measurement views: AM
Group	Fetch commands
Syntax	FETCH:AM:RESult?
Arguments	None
Returns	<+AM>, <-AM>, <Total AM> Where <+AM> ::= <NRf> is the positive peak modulation factor in percent (%). <-AM> ::= <NRf> is the negative peak modulation factor in percent (%). <Total AM> ::= <NRf> is the (peak to peak modulation factor)/2 in percent (%).
Examples	FETCH:AM:RESULT? might return 62.63, -50.89, 56.76.

FETCH:AVTime:AVERAge? (Query Only)

Returns the RMS (root-mean-square) value for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions	Measurement views: Amplitude versus Time
Group	Fetch commands

Syntax	FETCh:AVTime:AVERAge?
Arguments	None
Returns	<avg> : :=<NRF> is the RMS amplitude in dBm. The unit can be changed by the [SENSE]:POWer:UNITs command.
Examples	FETCh:AVTIME:AVERAGE? might return -2.53, indicating the RMS amplitude is -2.53 dBm.

FETCh:AVTime:{FIRSt|SECOnd|THIRd|FOURth}? (Query Only)

Returns the trace data in the Amplitude versus Time measurement.

The mnemonics FIRSt, SECOnd, THIRd, and FOURth represent Trace 1, Trace 2, Trace 3, and Math trace, respectively. The traces can be specified by the TRACe<x>:AVTime command subgroup.

Conditions	Measurement views: Amplitude versus Time
Group	Fetch commands
Syntax	FETCh:AVTime:{FIRSt SECOnd THIRd FOURth}?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude in dBm at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2. The unit can be changed by the [SENSE]:POWer:UNITs command.
Examples	FETCh:AVTIME:FIRST? might return #3156xxxx... (156-byte data) for Trace 1.

FETCh:AVTime:MAXimum? (Query Only)

Returns the maximum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions Measurement views: Amplitude versus Time

Group Fetch commands

Syntax FETCh:AVTime:MAXimum?

Related Commands [FETCh:AVTime:MAXLocation?](#)

Arguments None

Returns <max> ::= <Nrf> is the maximum Amplitude in dBm.
The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples FETCh:AVTIME:MAXIMUM? might return -2.84, indicating the maximum amplitude is -2.84 dBm.

FETCh:AVTime:MAXLocation? (Query Only)

Returns the time at which the amplitude is maximum for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions Measurement views: Amplitude versus Time

Group Fetch commands

Syntax FETCh:AVTime:MAXLocation?

Related Commands [FETCh:AVTime:MAXimum?](#)

Arguments None

Returns <max_time>::=<NRF> is the time at the maximum in seconds.

Examples FETCH:AVTIME:MAXLOCATION? might return 25.03E-9, indicating the amplitude is maximum at 25.03 ns.

FETCH:AVTime:MINimum? (Query Only)

Returns the minimum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions Measurement views: Amplitude versus Time

Group Fetch commands

Syntax FETCH:AVTime:MINimum?

Related Commands [FETCH:AVTime:MINLocation?](#)

Arguments None

Returns <min>::=<NRF> is the minimum amplitude in dBm.
The unit can be changed by the [\[SENSE\]:POWER:UNITs](#) command.

Examples FETCH:AVTIME:MINIMUM? might return -57.64, indicating the minimum amplitude is -57.64 dBm.

FETCH:AVTime:MINLocation? (Query Only)

Returns the time at which the amplitude is minimum for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions Measurement views: Amplitude versus Time

Group Fetch commands

Syntax FETCH:AVTime:MINLocation?

Related Commands	FETCh:AVTime:MINimum?
Arguments	None
Returns	<code><min_time>::=<NRf></code> is the time at the minimum in seconds.
Examples	<code>FETCH:AVTIME:MINLOCATION?</code> might return <code>450.7E-9</code> , indicating the amplitude is minimum at 450.7 ns.

FETCh:AVTime:RESult? (Query Only)

Returns the measurement results for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions	Measurement views: Amplitude versus Time
Group	Fetch commands
Syntax	<code>FETCh:AVTime:RESult?</code>
Arguments	None
Returns	<p><code><max>,<max_time>,<min>,<min_time>,<rms></code></p> <p>Where</p> <p><code><max>::=<NRf></code> is the maximum amplitude in dBm. <code><max_time>::=<NRf></code> is the time at the maximum in seconds. <code><min>::=<NRf></code> is the minimum amplitude in dBm. <code><min_time>::=<NRf></code> is the time at the minimum in seconds. <code><rms>::=<NRf></code> is the RMS amplitude in dBm. The unit of amplitude can be changed by the [SENSE]:POWER:UNITs command.</p>
Examples	<p><code>FETCH:AVTIME:RESULT?</code> might return <code>-2.68,48.62E-6,-82.47,22.11E-6,-8.24</code>, indicating that the maximum amplitude is -2.68 dBm at 48.62 μs, the minimum amplitude is -82.47 dBm at 22.11 μs, and the RMS amplitude is -8.24 dBm.</p>

FETCh:CCDF? (Query Only)

Returns the CCDF measurement results.

Conditions Measurement views: CCDF

Group Fetch commands

Syntax FETCh:CCDF?

Related Commands

Arguments None

Returns <avg_amp1>, <avg_ccdf>, <crest_factor>, <amp1_10>, <amp1_1>, <amp1_p1>, <amp1_p01>, <amp1_p001>, <amp1_p0001>

Where

<avg_amp1> is the average amplitude in dBm.

The unit can be changed by the [\[SENSE\]:POWER:UNITS](#) command.

<avg_ccdf> is the average CCDF in percent.

<crest_factor> is the crest factor in dB.

<amp1_10> is the amplitude at CCDF of 10% in dB.

<amp1_1> is the amplitude at CCDF of 1% in dB.

<amp1_p1> is the amplitude at CCDF of 0.1% in dB.

<amp1_p01> is the amplitude at CCDF of 0.01% in dB.

<amp1_p001> is the amplitude at CCDF of 0.001% in dB.

<amp1_p0001> is the amplitude at CCDF of 0.0001% in dB.

Examples FETCh:CCDF? might return
-33.35, 35.8, 9.75, 3.88, 7.07, 8.50, 9.25, 9.72, 9.74, indicating
(average amplitude) = -33.35 dBm,
(average CCDF) = 35.8%,
(crest factor) = 9.75 dB,
(amplitude at CCDF of 10%) = 3.88 dB,
(amplitude at CCDF of 1%) = 7.07 dB,
(amplitude at CCDF of 0.1%) = 8.50 dB,
(amplitude at CCDF of 0.01%) = 9.25 dB,
(amplitude at CCDF of 0.001%) = 9.72 dB, and
(amplitude at CCDF of 0.0001%) = 9.74 dB.

FETCh:CCDF:{FIRSt|SECond|THIRd}:X? (Query Only)

Returns the horizontal values of the specified trace in the CCDF measurement.

The mnemonics FIRSt, SECond, and THIRd represent Trace 1, Trace 2, and Gaussian reference curve, respectively.

Conditions Measurement views: CCDF

Group Fetch commands

Syntax FETCh:CCDF:{FIRSt|SECond|THIRd}:X?

Arguments None

Returns #<num_digit><num_byte><x(1)><x(2)>...<x(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<x(n)> is the horizontal value (dB) of the CCDF graph at the nth point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCh:CCDF:FIRSt:X? might return #41024xxxx... (1024-byte data) for the horizontal values of Trace 1.

FETCh:CCDF:{FIRSt|SECond|THIRd}:XY? (Query Only)

Returns the horizontal and vertical value pairs of the specified trace in the CCDF measurement.

The mnemonics FIRSt, SECond, and THIRd represent Trace 1, Trace 2, and Gaussian reference curve, respectively.

Conditions Measurement views: CCDF

Group Fetch commands

Syntax FETCh:CCDF:{FIRSt|SECond|THIRd}:XY?

Arguments	None
Returns	<p>#<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)>...<x(n)><y(n)></p> <p>Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)><y(n)> is the horizontal value (dB) and vertical value (%) pair at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.</p>
Examples	<p>FETCH:CCDF:FIRST:XY? might return #41024xxxx... (1024-byte data) for the horizontal and vertical value pairs of Trace 1.</p>

FETCh:CCDF:{FIRSt|SECOnd|THIRd}[:Y]? (Query Only)

Returns the vertical values of the specified trace in the CCDF measurement.

The mnemonics FIRSt, SECOnd, and THIRd represent Trace 1, Trace 2, and Gaussian reference curve, respectively.

Conditions	Measurement views: CCDF
Group	Fetch commands
Syntax	FETCH:CCDF:{FIRSt SECOnd THIRd}[:Y]?
Arguments	None
Returns	<p>#<num_digit><num_byte><y(1)><y(2)>...<y(n)></p> <p>Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <y(n)> is the vertical value (%) of the CCDF graph at the nth point, 4-byte little endian floating-point format specified in IEEE 488.2.</p>
Examples	<p>FETCH:CCDF:FIRST:Y? might return #41024xxxx... (1024-byte data) for the vertical values of Trace 1.</p>

FETCh:CONStE:FERRor? (Query Only)

Returns the frequency error in Hz. The frequency error is the difference between the measured carrier frequency of the signal and the user-selected center frequency of the analyzer.

Group Fetch commands

Syntax FETCh:CONStE:FERRor?

Related Commands [FETCh:EVM:FERRor?](#)

Arguments None.

Returns <freq_error>::=<Nrf> which is the frequency error in Hz.

Examples FETCh:CONStE:? might return -10.7E+3, which is a frequency error of -10.7 kHz.

FETCh:CONStE:RESuLts? (Query Only)

Returns the constellation measurement results of EVM RMS, peak and location displayed on the bottom of the screen.

Conditions Measurement views: Constellation

Group Fetch commands

Syntax FETCh:CONStE:RESuLts?

Arguments None

Returns For modulation types 2|4|8|16FSK or C4FM:
FSK_deviation_Avg_Leftmost, FSK_deviation_Avg_Rightmost
Where
FSK_deviation_Avg_Leftmost is the average FSK deviation of the left-most symbol in Hz.

FSK_deviation_Avg_Rightmost is the average FSK deviation of the right-most symbol in Hz.

For all other valid modulation types:

<EVM_RMS>, <EVM_peak>, <location>

Where

<EVM_RMS> ::= <NRf> is the RMS EVM in percent (%).

<EVM_peak> ::= <NRf> is the peak EVM in percent (%).

<location> ::= <NRf> is the peak location in symbol number.

The time unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.

Examples FETCH:CONStE:RESUlTS? might return 2.841, 3.227, 68.000, indicating that the RMS EVM is 2.841% and the peak EVM is 3.227% at symbol #68.

FETCh:CONStE:TRACe? (Query Only)

Returns the constellation trace data.

Conditions Measurement views: Constellation

Group Fetch commands

Syntax FETCh:CONStE:TRACe?

Arguments None

Returns #<num_digit><num_byte><I(1)><Q(1)><I(2)><Q(2)> . . .
<I(n)><Q(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<I(n)> and <Q(n)> are the normalized I- and Q-coordinate values at the nth data point. 4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCH:CONStE:TRACe? might return #43848xxxx . . . (3848-byte data) for the constellation trace data.

FETCh:DDEMod:STABle? (Query Only)

Returns the symbol table data.

Conditions Measurement views: Symbol table

Group Fetch commands

Syntax FETCh:DDEMod:STABle?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the symbol table data at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCh:DDEMOD:STABLE? might return #3512xxxx... (512-byte data) for the symbol table.

FETCh:DDEMod:SYNCh:WORD:LENGth? (Query Only)

Returns the length of the synch word in the symbol table.

Conditions Measurement views: Symbol table

Group Fetch commands

Syntax FETCh:DDEMod:SYNCh:WORD:LENGth?

Related Commands [FETCh:DDEMod:SYNCh:WORD:POSition?](#)

Arguments None

Returns <NR1> indicates the length of the synch word in symbols.

Examples `FETCH:DDEMOD:SYNCH:WORD:LENGTH?` might return 3, indicating the length of the synch word is three symbols.

FETCH:DDEMod:SYNCh:WORD:POSition? (Query Only)

Returns the position of the synch word in the symbol table.

Conditions Measurement views: Symbol table

Group Fetch commands

Syntax `FETCH:DDEMod:SYNCh:WORD:POSition?`

Related Commands [FETCH:DDEMod:SYNCh:WORD:LENGth?](#)

Arguments None

Returns <NR1> indicates what symbol number the synch word begins at in the table. Zero (0) represents the first symbol in the table. A “-1” indicates that the synch word was not found.

Examples `FETCH:DDEMOD:SYNCH:WORD:POSITION?` might return 10, indicating the synch word begins at 11th symbol in the table.

FETCH:DIQVtime:FERRor? (Query Only)

Returns the frequency error in the Demod I&Q versus Time measurement.

Conditions Measurement views: Demod I&Q versus Time

Group Fetch commands

Syntax `FETCH:DIQVtime:FERRor?`

Arguments None

Returns <freq_error> ::= <NRf> is the frequency error in Hz.

Examples FETCH:DIQVTIME:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:DIQVtime:I? (Query Only)

Returns the I versus Time trace data.

Conditions Measurement views: Demod I&Q versus Time

Group Fetch commands

Syntax FETCh:DIQVtime:I?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the I level in volts at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCH:DIQVTIME:I? might return #3160xxxx... (160-byte data) for the I versus Time trace.

FETCh:DIQVtime:Q? (Query Only)

Returns the Q versus Time trace data.

Conditions Measurement views: Demod I&Q versus Time

Group Fetch commands

Syntax FETCh:DIQVtime:Q?

Arguments	None
Returns	<code>#<num_digit><num_byte><data(1)><data(2)>...<data(n)></code> Where <code><num_digit></code> is the number of digits in <code><num_byte></code> . <code><num_byte></code> is the number of bytes of data that follow. <code><data(n)></code> is the Q level in volts at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	<code>FETCH:DIQVTIME:Q?</code> might return <code>#3160xxx...</code> (160-byte data) for the Q versus Time trace.

FETCH:DPSA:RESULTS:TRACE<x>? (Query Only)

Returns waveform data of specified trace `<x>` in the DPX spectrum measurement, where `x` is 1 to 5. The traces 1–4 are in the standard form. Trace 5 is the bitmap trace and its data is returned in a binary block.

Conditions	Measurement views: DPX spectrum
Group	Fetch commands
Syntax	<code>FETCH:DPSA:RESULTS:TRACE<x>?</code>
Arguments	<code><NR1></code>
Returns	For traces 1 to 4: <code>#<num_digit><num_byte><data(1)><data(2)>...<data(n)></code> Where <code><num_digit></code> is the number of digits in <code><num_byte></code> . <code><num_byte></code> is the number of bytes of data that follow. <code><data(n)></code> is the amplitude of the trace sample at the n^{th} data point. <code><data(n)></code> is in the 4-byte little endian floating-point format specified in IEEE 488.2. For trace 5, the format differs depending on whether Option 200 is installed in the instrument. Without Option 200, the format is a binary block of unsigned 16 bit integers. Each value ranges from 0 to $2^{16}-1$, where $2^{16}-1$ represents 100%.

With Option 200, the format is a binary block of 32 bit floating point values. Each value ranges from 0 to 1.0, where 1.0 represents 100%.

Examples `FETCh:DPSA:RESuLts:TRACe1?` might return `#42004xxxx...` (2004-byte of data) for the waveform data of trace one (1).

FETCh:DPSA:TRACe:AVERAge? (Query Only)

Returns waveform data of the average trace in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Fetch commands

Syntax `FETCh:DPSA:TRACe:AVERAge?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the amplitude of the average trace at the n^{th} data point in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `FETCh:DPSA:TRACe:AVERAGE?` might return `#42004xxxx...` (2004-byte data) for the waveform data of the average trace.

FETCh:DPSA:TRACe:BITMap? (Query Only)

Returns a data block of the DPX spectrum measurement bitmap waveform data.

Conditions Measurement views: DPX spectrum

Group Fetch commands

Syntax **FETCH:DPSA:TRACe:BITMap?**

Arguments None

Returns (With Option 200) A binary block of 32-bit floating point values (IEEE standard single precision floating point format). Each value ranges from 0 to 1.0, where 1.0 represents 100%. Option 200 bitmaps have 201 rows and 801 columns. Data[0] is the first column in the first row, data[801] is the first column in the 2nd row, and so on.

(Without Option 200) A binary block of unsigned 16-bit Little Endian integers. Each value ranges from 0 to $2^{16}-1$, where $2^{16}-1$ represents 100%. Non-option-200 bitmaps have 201 rows and 501 columns. Data[0] is the first column in the first row, data[501] is the first column in the 2nd row, and so on.

Examples **FETCH:DPSA:TRACe:BITMAP?** might return #6644004xxxx... (Option 200) or #161,001xxxx... (non-Option 200).

FETCH:DPSA:TRACe:MATH? (Query Only)

Returns waveform data of the math trace in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Fetch commands

Syntax **FETCH:DPSA:TRACe:MATH?**

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude of the math trace at the nth data point in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the **[SENSe]:POWer:UNITs** command.

Examples `FETCH:DPSA:TRACE:MATH?` might return `#42004xxxx...` (2004-byte data) for the waveform data of the math trace.

FETCH:DPSA:TRACe:MAXimum? (Query Only)

Returns waveform data of the maximum trace in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Fetch commands

Syntax `FETCH:DPSA:TRACe:MAXimum?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the amplitude of the maximum trace at the n^{th} data point in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `FETCH:DPSA:TRACE:MAXIMUM?` might return `#42004xxxx...` (2004-byte data) for the waveform data of the maximum trace.

FETCH:DPSA:TRACe:MINimum? (Query Only)

Returns waveform data of the minimum trace in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Fetch commands

Syntax `FETCH:DPSA:TRACe:MINimum?`

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude data of the minimum trace at the nth data point in dBm,

4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSE\]:POWER:UNITS](#) command.

Examples FETCH:DPSA:TRACE:MINIMUM? might return #42004xxxx... (2004-byte data) for the waveform data of the minimum trace.

FETCh:EDiagram:FDEVIation? (Query Only)

Returns the frequency deviation versus Time trace data with the X values.

Group Fetch commands

Syntax FETCh:EDIagram:FDEVIation?

Related Commands

Returns #<num_digit><num_byte><Y(1)><X(1)><Y(2)><X(2)>...<Y(n)><X(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<Y(n)> and <X(n)> is the frequency deviation in Hz and time (symbols) pair at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCH:EDIAGRAM:FDEVIATION? might return #3160xxxx... (160-byte data) for the frequency deviation versus Time trace.

FETCh:EDiagram:FERRor? (Query Only)

Returns the frequency error in the eye diagram measurement.

Conditions Measurement views: Eye diagram

Group	Fetch commands
Syntax	FETCh:EDIagram:FERRor?
Arguments	None
Returns	<freq_error> := <NRF> is the frequency error in Hz.
Examples	FETCh:EDIAGRAM:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:EDIagram:I? (Query Only)

Returns the I versus Time trace data in the eye diagram measurement.

Conditions	Measurement views: Eye diagram
Group	Fetch commands
Syntax	FETCh:EDIagram:I?
Arguments	None
Returns	#<num_digit><num_byte><Y(1)><X(1)><Y(2)><X(2)>...<Y(n)><X(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <Y(n)><X(n)> is the I level (normalized) and time (symbols) pair at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	FETCh:EDIAGRAM:I? might return #3160xxxx... (160-byte data) for the I versus Time trace.

FETCh:EDIagram:Q? (Query Only)

Returns the Q versus Time trace data in the eye diagram measurement.

Conditions	Measurement views: Eye diagram
Group	Fetch commands
Syntax	FETCh:EDIagram:Q?
Arguments	None
Returns	#<num_digit><num_byte><Y(1)><X(1)><Y(2)><X(2)>...<Y(n)><X(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <Y(n)><X(n)> is the Q level (normalized) and time (symbols) pair at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	FETCh:EDIAGRAM:Q? might return #3160xxxx... (160-byte data) for the Q versus Time trace.

FETCh:EVM:FERRor? (Query Only)

Returns the frequency error in the EVM versus Time measurement.

Conditions	Measurement views: EVM versus Time
Group	Fetch commands
Syntax	FETCh:EVM:FERRor?
Arguments	None
Returns	<freq_error>::=<Nrf> is the frequency error in Hz.
Examples	FETCh:EVM:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:EVM:PEAK? (Query Only)

Returns the peak value in the EVM versus Time measurement.

Conditions Measurement views: EVM versus Time

Group Fetch commands

Syntax FETCh:EVM:PEAK?

Related Commands [FETCh:EVM:PINdex?](#)

Arguments None

Returns <peak> ::= <Nrf> is the peak EVM value in percent (%).

Examples FETCh:EVM:PEAK? might return 1.32, indicating the peak EVM value is 1.32%.

FETCh:EVM:PINdex? (Query Only)

Returns the time at the EVM peak.

Conditions Measurement views: EVM versus Time

Group Fetch commands

Syntax FETCh:EVM:PINdex?

Related Commands [FETCh:EVM:PEAK?](#)

Arguments None

Returns <peak_time> ::= <Nrf> is the time at the EVM peak in symbol number. The unit can be changed by the [\[SENSE\]:DDEMod:TIME:UNITs](#) command.

Examples `FETCH:EVM:PINDEX?` might return `68.000`, indicating that the EVM peak is at symbol #68.

FETCH:EVM:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the EVM versus Time measurement.

Conditions Measurement views: EVM versus Time

Group Fetch commands

Syntax `FETCH:EVM:RMS?`

Arguments None

Returns `<rms>::=<NRF>` is the RMS EVM value in percent (%).

Examples `FETCH:EVM:RMS?` might return `0.582`, indicating the RMS EVM value is 0.582%.

FETCH:EVM:TRACe? (Query Only)

Returns the EVM versus Time trace data.

Conditions Measurement views: EVM versus Time

Group Fetch commands

Syntax `FETCH:EVM:TRACe?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where
`<num_digit>` is the number of digits in `<num_byte>`.

<num_byte> is the number of bytes of data that follow.
<data(n)> is the EVM value at the nth data point in percent (%),
4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:EVM:TRACE?` might return `#42036xxxx...` (2036-byte data) for the EVM versus Time trace.

FETCH:FDVTime:FERRor? (Query Only)

Returns the frequency error in the Frequency deviation versus Time measurement.

Conditions Measurement views: Frequency deviation versus Time

Group Fetch commands

Syntax `FETCH:FDVTime:FERRor?`

Arguments None

Returns <freq_error>::=<Nrf> is the frequency error in Hz.

Examples `FETCH:FDVTime:FERRor?` might return `-10.7E+3`, indicating the frequency error is -10.7 kHz.

FETCH:FDVTime:TRACe? (Query Only)

Returns the Frequency deviation versus Time trace data.

Conditions Measurement views: Frequency deviation versus Time

Group Fetch commands

Syntax `FETCH:FDVTime:TRACe?`

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the frequency deviation in Hz at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCH:FDVTIME:TRACE? might return #3160xxxx... (160-byte data) for the Frequency deviation versus Time trace.

FETCh:{FM|PM}:FERRor? (Query Only)

Returns the frequency error in the Frequency modulation or Phase modulation measurements.

Conditions Measurement views: Frequency deviation versus Time

Group Fetch commands

Syntax FETCh:{FM|PM}:FERRor?

Arguments None

Returns <freq_error>::=<Nrf> is the frequency error in Hz.

Examples FETCh:{FM|PM}:FERRor? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:FM:PHALf? (Query Only)

Returns the half peak-peak frequency deviation (Pk-Pk/2) in the FM measurement.

Conditions Measurement views: FM

Group Fetch commands

Syntax FETCh:FM:PHALf?

Arguments	None
Returns	<Pk-Pk/2> := <NRf> is the half peak-peak frequency deviation in Hz.
Examples	FETCH:FM:PHALF? might return 628.9E+3, indicating the half peak-peak frequency deviation is 628.9 kHz.

FETCH:FM:PNEGative? (Query Only)

Returns the negative peak frequency deviation ($-Pk$) in the FM measurement.

Conditions	Measurement views: FM
Group	Fetch commands
Syntax	FETCH:FM:PNEGative?
Arguments	None
Returns	<-Pk> := <NRf> is the negative peak frequency deviation in Hz.
Examples	FETCH:FM:PNEGATIVE? might return -495.6E+3, indicating the negative peak frequency deviation is -495.6 kHz.

FETCH:FM:PPOSitive? (Query Only)

Returns the positive peak frequency deviation ($+Pk$) in the FM measurement.

Conditions	Measurement views: FM
Group	Fetch commands
Syntax	FETCH:FM:PPOSitive?
Arguments	None

Returns <+Pk> ::= <Nrf> is the positive peak frequency deviation in Hz.

Examples FETCH:FM:PPOSITIVE? might return 763.2E+3, indicating the positive peak frequency deviation is 763.2 kHz.

FETCh:FM:PTPeak? (Query Only)

Returns the peak-peak frequency deviation (Pk-Pk) in the FM measurement.

Conditions Measurement views: FM

Group Fetch commands

Syntax FETCh:FM:PTPeak?

Arguments None

Returns <Pk-Pk> ::= <Nrf> is the peak-peak frequency deviation in Hz.

Examples FETCH:FM:PTPEAK? might return 1.258E+6, indicating the peak-peak frequency deviation is 1.258 MHz.

FETCh:FM:RESult? (Query Only)

Returns the FM measurement results.

Conditions Measurement views: FM

Group Fetch commands

Syntax FETCh:FM:RESult?

Arguments None

Returns <+Pk>, <-Pk>, <RMS>, <Pk-Pk>, <Pk-Pk/2>

Where

<+Pk> ::= <NRf> is the positive peak frequency deviation in Hz.

<-Pk> ::= <NRf> is the negative peak frequency deviation in Hz.

<RMS> ::= <NRf> is the RMS frequency deviation in Hz.

<Pk-Pk> ::= <NRf> is the peak-peak frequency deviation in Hz.

<Pk-Pk/2> ::= <NRf> is the half peak-peak frequency deviation in Hz.

Examples `FETCH:FM:RESULT?` might return
763.2E+3, -494.6E+3, 271.2E+3, 1.258E+6, 628.9E+3.

FETCH:FM:RMS? (Query Only)

Returns the RMS frequency deviation in the FM measurement.

Conditions Measurement views: FM

Group Fetch commands

Syntax `FETCH:FM:RMS?`

Arguments None

Returns <RMS> ::= <NRf> is the RMS frequency deviation in Hz.

Examples `FETCH:FM:RMS?` might return 271.2E+3, indicating the RMS frequency deviation is 271.2 kHz.

FETCH:FVTime? (Query Only)

Returns the Frequency versus Time trace data.

Conditions Measurement views: Frequency versus Time

Group Fetch commands

Syntax `FETCH:FVTime?`

Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the frequency in Hz at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	FETCH:FVTIME? might return #3156xxxx... (156-byte data) for the Frequency versus Time trace.

FETCH:FVTime:MAXimum? (Query Only)

Returns the maximum value in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Fetch commands
Syntax	FETCH:FVTime:MAXimum?
Related Commands	FETCH:FVTime:MAXLocation?
Arguments	None
Returns	<max> ::= <NRF> is the maximum frequency drift in Hz.
Examples	FETCH:FVTIME:MAXIMUM? might return 2.625E+6, indicating the maximum frequency drift is 2.625 MHz.

FETCH:FVTime:MAXLocation? (Query Only)

Returns the time at which the frequency drift is maximum.

Conditions	Measurement views: Frequency versus Time
-------------------	--

Group	Fetch commands
Syntax	FETCH:FVTime:MAXLocation?
Related Commands	FETCH:FVTime:MAXimum?
Arguments	None
Returns	<max_time>::=<NRf> is the time in seconds at which the frequency drift is maximum.
Examples	FETCH:FVTIME:MAXLOCATION? might return 25.03E-9, indicating the frequency drift is maximum at 25.03 ns.

FETCH:FVTime:MINimum? (Query Only)

Returns the minimum value in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Fetch commands
Syntax	FETCH:FVTime:MINimum?
Related Commands	FETCH:FVTime:MINLocation?
Arguments	None
Returns	<min>::=<NRf> is the minimum frequency drift in Hz.
Examples	FETCH:FVTIME:MINIMUM? might return -6.618E+6, indicating the minimum frequency drift is -6.618 MHz.

FETCH:FVTime:MINLocation? (Query Only)

Returns the time at which the frequency drift is minimum.

Conditions	Measurement views: Frequency versus Time
Group	Fetch commands
Syntax	<code>FETCh:FVTime:MINLocation?</code>
Related Commands	FETCh:FVTime:MINimum?
Arguments	None
Returns	<code><min_time>::=<NRf></code> is the time in seconds at which the frequency drift is minimum.
Examples	<code>FETCH:FVTIME:MINLOCATION?</code> might return <code>450.7E-9</code> , indicating the frequency drift is minimum at 450.7 ns.

FETCh:FVTime:RESult? (Query Only)

Returns the Frequency versus Time measurement results.

Conditions	Measurement views: Frequency versus Time
Group	Fetch commands
Syntax	<code>FETCh:FVTime:RESult?</code>
Arguments	None
Returns	<code><max>, <max_time>, <min>, <min_time></code> Where <code><max>::=<NRf></code> is the maximum frequency drift in Hz. <code><max_time>::=<NRf></code> is the time in seconds at which the frequency drift is maximum. <code><min>::=<NRf></code> is the minimum frequency drift in Hz. <code><min_time>::=<NRf></code> is the time in seconds at which the frequency drift is minimum.

Examples `FETCH:FVTIME:RESULT?` might return `2.625E+6,25.03E-9,-6.618E+6,450.7E-9`, indicating the maximum frequency drift is 2.625 MHz at 25.03 ns and the minimum frequency drift is -6.618 MHz at 450.7 ns.

FETCH:IQVTime:I? (Query Only)

Returns the I versus Time trace data.

Conditions Measurement views: RF I&Q versus Time

Group Fetch commands

Syntax `FETCH:IQVTime:I?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the I level in volts at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:IQVTIME:I?` might return `#3160xxxx...` (160-byte data) for the I versus Time trace.

FETCH:IQVTime:MAXimum? (Query Only)

Returns the maximum value in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Fetch commands

Syntax `FETCH:IQVTime:MAXimum?`

Related Commands	FETCh:IQVTime:MAXLocation?
Arguments	None
Returns	<p><max>::=<Nrf> is the maximum I or Q level in volts.</p> <p>Use the TRACe:IQVTime:SElect:I or TRACe:IQVTime:SElect:Q command to select the trace.</p>
Examples	FETCh:IQVTime:MAXIMUM? might return 1.214, indicating the maximum I or Q level is 1.214 V.

FETCh:IQVTime:MAXLocation? (Query Only)

Returns the time at which the I or Q level is maximum.

Conditions	Measurement views: RF I&Q versus Time
Group	Fetch commands
Syntax	FETCh:IQVTime:MAXLocation?
Related Commands	FETCh:IQVTime:MAXimum?
Arguments	None
Returns	<max_time>::=<Nrf> is the time in seconds at which the I or Q level is maximum.
Examples	FETCh:IQVTime:MAXLOCATION? might return 175.3E-9, indicating the I or Q level is maximum at 175.3 ns.

FETCh:IQVTime:MINimum? (Query Only)

Returns the minimum value in the RF I&Q versus Time measurement.

Conditions	Measurement views: RF I&Q versus Time
-------------------	---------------------------------------

Group	Fetch commands
Syntax	<code>FETCh:IQVTime:MINimum? imum</code>
Related Commands	FETCh:IQVTime:MINLocation?
Arguments	None
Returns	<code><min>::=<Nrf></code> is the minimum I or Q level in volts. Use the TRACe:IQVTime:SElect:I or TRACe:IQVTime:SElect:Q command to select the trace.
Examples	<code>FETCh:IQVTime:MINimum?</code> might return <code>-370.5E-3</code> , indicating the minimum I or Q level is -370.5 mV.

FETCh:IQVTime:MINLocation? (Query Only)

Returns the time at which the I or Q level is minimum.

Conditions	Measurement views: RF I&Q versus Time
Group	Fetch commands
Syntax	<code>FETCh:IQVTime:MINLocation?</code>
Related Commands	FETCh:IQVTime:MINimum?
Arguments	None
Returns	<code><min_time>::=<Nrf></code> is the time in seconds at which the I or Q level is minimum.
Examples	<code>FETCh:IQVTime:MINLOCATION?</code> might return <code>450.7E-9</code> , indicating the I or Q level is minimum at 450.7 ns.

FETCh:IQVTime:Q? (Query Only)

Returns the Q versus Time trace data.

Conditions	Measurement views: RF I&Q versus Time
Group	Fetch commands
Syntax	FETCh:IQVTime:Q?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the Q level in volts at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	FETCh:IQVTime:Q? might return #3160xxxx... (160-byte data) for the Q versus Time trace.

FETCh:IQVTime:RESult? (Query Only)

Returns the RF I&Q versus Time measurement results.

Conditions	Measurement views: RF I&Q versus Time
Group	Fetch commands
Syntax	FETCh:IQVTime:RESult?
Arguments	None
Returns	<max>, <max_time>, <min>, <min_time> Where <max> ::= <Nrf> is the maximum I or Q level in volts.

`<max_time>::=<Nrf>` is the time in seconds at which the I or Q level is maximum.

`<min>::=<Nrf>` is the minimum I or Q level in volts.

`<min_time>::=<Nrf>` is the time in seconds at which the I or Q level is minimum.

Use the [TRACe:IQVTime:SElect:I](#) or [TRACe:IQVTime:SElect:Q](#) command to select the trace.

Examples `FETCH:IQVTIME:RESULT?` might return `1.214,175.3E-9,-370.5E-3,450.7E-9`, indicating the maximum I or Q level is 1.214 V at 175.3 ns and the minimum I or Q level is -370.5 mV at 450.7 ns.

FETCh:MCPower:ADJacent:CHANnels? (Query Only)

Returns the power of adjacent channels in order of increasing frequency.

Conditions Measurement views: MCPR

Group Fetch commands

Syntax `FETCh:MCPower:ADJacent:CHANnels?`

Arguments None

Returns `<acpr_lower(n)>, ... <acpr_lower(2)>, <acpr_lower(1)>, <acpr_upper(1)>, <acpr_upper(2)>, ... <acpr_upper(n)>`

Where

`<acpr_lower(n)>` is the ACPR for the lower channel #n in dB.

`<acpr_upper(n)>` is the ACPR for the upper channel #n in dB.

To add a pair of upper and lower adjacent channels, use the [\[SENSe\]:MCPower:CHANnel:ADJacent:ADD](#) command.

Examples `FETCH:MCPOWER:ADJACENT:CHANNELS?` might return `-4.420,-4.847,-4.316,-4.225`, indicating (ACPR for the lower channel 2) = -4.420 dB, (ACPR for the lower channel 1) = -4.847 dB, (ACPR for the upper channel 1) = -4.316 dB, and (ACPR for the upper channel 2) = -4.225 dB.

FETCh:MCPower:CHANnel:POWer? (Query Only)

Returns the reference power in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Fetch commands
Syntax	FETCh:MCPower:CHANnel:POWer?
Arguments	None
Returns	<p><ref_power>: <Nrf> is the reference power in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.</p> <p>To select the power reference, use the [SENSe]:MCPower:RCHannels? commands.</p>
Examples	FETCh:MCPOWER:CHANNEL:POWER? might return 4.227, indicating that the reference power is 4.227 dBm.

FETCh:MCPower:MAIN:CHANnels? (Query Only)

Returns the power of main channels in order of increasing frequency.

Conditions	Measurement views: MCPR
Group	Fetch commands
Syntax	FETCh:MCPower:MAIN:CHANnels?
Arguments	None
Returns	<p><power_main(1)>, <power_main(2)>, ... <power_main(n)></p> <p>Where <power_main(n)> is the power of main channel #n in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.</p>

To specify the main channels, use the [SENSe]:MCPower:CHANnel:MAIN commands.

Examples `FETCH:MCPOWER:MAIN:CHANNELS?` might return `-2.420,-2.847,-2.316,-2.225`, indicating
 (power of the main channel 1) = -2.420 dBm,
 (power of the main channel 2) = -2.847 dBm,
 (power of the main channel 3) = -2.316 dBm, and
 (power of the main channel 4) = -2.225 dBm.

FETCH:MCPower:SPECTrum? (Query Only)

Returns spectrum trace data of the MCPR measurement.

Conditions Measurement views: MCPR

Group Fetch commands

Syntax `FETCH:MCPOWER:SPECTrum?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the amplitude in dBm at the n^{th} data point,

4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [SENSe]:POWER:UNITs command.

Examples `FETCH:MCPOWER:SPECTRUM?` might return `#43204xxxx...` (3204-byte data)
 for the spectrum trace data of the MCPR measurement.

FETCH:MERRor:FERRor? (Query Only)

Returns the frequency error in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group	Fetch commands
Syntax	FETCh:MERRor:FERRor?
Arguments	None
Returns	<freq_error> ::= <NRf> is the frequency error in Hz.
Examples	FETCh:MERRor:FERRor? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:MERRor:PEAK? (Query Only)

Returns the peak value in the Magnitude error versus Time measurement.

Conditions	Measurement views: Magnitude error versus Time
Group	Fetch commands
Syntax	FETCh:MERRor:PEAK?
Related Commands	FETCh:MERRor:PINdex?
Arguments	None
Returns	<peak> ::= <NRf> is the peak magnitude error in percent (%).
Examples	FETCh:MERRor:PEAK? might return 1.57, indicating the peak magnitude error is 1.57%.

FETCh:MERRor:PINdex? (Query Only)

Returns the time at the magnitude error peak.

Conditions	Measurement views: Magnitude error versus Time
-------------------	--

Group	Fetch commands
Syntax	FETCh:MERRor:PINDEx?
Related Commands	FETCh:MERRor:PEAK?
Arguments	None
Returns	<peak_time>::=<NRf> is the time at the magnitude error peak in symbol number. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	FETCh:MERRor:PINDEx? might return 68.000, indicating that the magnitude error peak is at symbol #68.

FETCh:MERRor:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Fetch commands

Syntax FETCh:MERRor:RMS?

Arguments None

Returns <rms>::=<NRf> is the RMS magnitude error in percent (%).

Examples FETCh:MERRor:RMS? might return 0.382, indicating the magnitude error is 0.382% RMS.

FETCh:MERRor:TRACe? (Query Only)

Returns the Magnitude error versus Time trace data.

Conditions	Measurement views: Magnitude error versus Time
Group	Fetch commands
Syntax	FETCH:MERROR:TRACE?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the magnitude error in percent (%) at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	FETCH:MERROR:TRACE? might return #42036xxxx... (2036-byte data) for the Magnitude error versus Time trace.

FETCH:OBWidth:FREQUENCY:ERROR? (Query Only)

Returns the frequency error in the Occupied Bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Fetch commands
Syntax	FETCH:OBwidth:FREQUENCY:ERROR?
Arguments	None
Returns	<freq_error>::=<NRF> is the frequency error in Hz.
Examples	FETCH:OBWIDTH:FREQUENCY:ERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:OBWidth:OBWidth:BANDwidth? (Query Only)

Returns the occupied bandwidth in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax FETCh:OBWidth:OBWidth:BANDwidth?

Arguments None

Returns <OBW> ::= <NRf> is the occupied bandwidth in Hz.

Examples FETCh:OBWidth:OBWidth:BANDwidth? might return 4.0E+6, indicating the occupied bandwidth is 4 MHz.

FETCh:OBWidth:OBWidth:LEFT:FREQUENCY? (Query Only)

Returns the left (lower) frequency of the occupied bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax FETCh:OBWidth:OBWidth:LEFT:FREQUENCY?

Related Commands [FETCh:OBWidth:OBWidth:RIGHT:FREQUENCY?](#)

Arguments None

Returns <OBW_left_freq> ::= <NRf> is the left frequency in Hz.

Examples FETCh:OBWidth:OBWidth:LEFT:FREQUENCY? might return 1.498E+9, indicating the left frequency is 1.498 GHz.

FETCh:OBWidth:OBWidth:LEFT:LEVel? (Query Only)

Returns the level at the left frequency of the occupied bandwidth.

Conditions	Measurement views: Occupied Bandwidth
Group	Fetch commands
Syntax	FETCh:OBWidth:OBWidth:LEFT:LEVel?
Related Commands	FETCh:OBWidth:OBWidth:RIGHT:LEVel?
Arguments	None
Returns	<OBW_left_level>::=<NRf> is the level at the left frequency in dB.
Examples	FETCh:OBWidth:OBWidth:LEFT:LEVel? might return -23.5, indicating the level at the left frequency is -23.5 dB.

FETCh:OBWidth:OBWidth:POWer? (Query Only)

Returns the reference power in the Occupied Bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Fetch commands
Syntax	FETCh:OBWidth:OBWidth:POWer?
Arguments	None
Returns	<OBW_ref_power>::=<NRf> is the reference power in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	FETCh:OBWidth:OBWidth:POWer? might return -10.0, indicating the reference power is -10 dBm.

FETCh:OBWidth:OBWidth:RIGHT:FREQUENCY? (Query Only)

Returns the right (higher) frequency of the occupied bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax FETCh:OBWidth:OBWidth:RIGHT:FREQUENCY?

Related Commands [FETCh:OBWidth:OBWidth:LEFT:FREQUENCY?](#)

Arguments None

Returns <OBW_right_freq>::=<Nrf> is the right frequency in Hz.

Examples FETCh:OBWidth:OBWidth:RIGHT:FREQUENCY? might return 1.502E+9, indicating the right frequency is 1.502 GHz.

FETCh:OBWidth:OBWidth:RIGHT:LEVel? (Query Only)

Returns the level at the right frequency of the occupied bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax FETCh:OBWidth:OBWidth:RIGHT:LEVel?

Related Commands [FETCh:OBWidth:OBWidth:LEFT:LEVel?](#)

Arguments None

Returns <OBW_right_level>::=<Nrf> is the level at the right frequency in dB.

Examples `FETCH:OBWIDTH:OBWIDTH:RIGHT:LEVEL?` might return `-23.5`, indicating the level at the right frequency is `-23.5` dB.

FETCH:OBWidth:SPECTrum? (Query Only)

Returns spectrum trace data of the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax `FETCH:OBwidth:SPECTrum?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the amplitude in dBm at the n^{th} data point,

4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the `[SENSE]:POWER:UNITs` command.

Examples `FETCH:OBWIDTH:SPECTRUM?` might return `#43204xxxx...` (3204-byte data) for the spectrum trace data of the Occupied Bandwidth measurement.

FETCH:OBWidth:XDBBandwidth:BANDwidth? (Query Only)

Returns the x dB bandwidth in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax `FETCH:OBwidth:XDBBandwidth:BANDwidth?`

Arguments None

Returns <xdBW> ::= <Nrf> is the x dB bandwidth in Hz.

Examples FETCH:OBWIDTH:XDBBANDWIDTH:BANDWIDTH? might return 2.0E+6, indicating the x dB bandwidth is 2 MHz.

FETCH:OBWidth:XDBBandwidth:LEFT:FREQUENCY? (Query Only)

Returns the left (lower) frequency of the x dB bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax FETCH:OBWidth:XDBBandwidth:LEFT:FREQUENCY?

Related Commands [FETCH:OBWidth:XDBBandwidth:RIGHT:FREQUENCY?](#)

Arguments None

Returns <xdBW_left_freq> ::= <Nrf> is the left frequency in Hz.

Examples FETCH:OBWIDTH:XDBBANDWIDTH:LEFT:FREQUENCY? might return 1.498E+9, indicating the left frequency is 1.498 GHz.

FETCH:OBWidth:XDBBandwidth:LEFT:LEVEL? (Query Only)

Returns the level at the left frequency of the x dB bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax FETCH:OBWidth:XDBBandwidth:LEFT:LEVEL?

Related Commands [FETCH:OBWidth:XDBBandwidth:RIGHT:LEVEL?](#)

Arguments	None
Returns	<xdbbw_left_level>::=<NRF> is the level at the left frequency in dB.
Examples	FETCH:OBWIDTH:XDBBANDWIDTH:LEFT:LEVEL? might return -23.5, indicating the level at the left frequency is -23.5 dB.

FETCH:OBWidth:XDBBandwidth:POWER? (Query Only)

Returns the reference power in the x dB bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Fetch commands
Syntax	FETCH:OBWidth:XDBBandwidth:POWER?
Arguments	None
Returns	<xdbbw_ref_power>::=<NRF> is the reference power in dBm. The unit can be changed by the [SENSE]:POWER:UNITS command.
Examples	FETCH:OBWIDTH:XDBBANDWIDTH:POWER? might return -10.0, indicating the reference power is -10 dBm.

FETCH:OBWidth:XDBBandwidth:RIGHT:FREQUENCY? (Query Only)

Returns the right (higher) frequency of the x dB bandwidth.

Conditions	Measurement views: Occupied Bandwidth
Group	Fetch commands
Syntax	FETCH:OBWidth:XDBBandwidth:RIGHT:FREQUENCY?
Related Commands	FETCH:OBWidth:XDBBandwidth:LEFT:FREQUENCY?

Arguments	None
Returns	<xdBW_right_freq>::=<NRF> is the right frequency in Hz.
Examples	FETCH:OBWIDTH:XDBBANDWIDTH:RIGHT:FREQUENCY? might return 1.502E+9, indicating the right frequency is 1.502 GHz.

FETCH:OBWidth:XDBBandwidth:RIGHT:LEVEL? (Query Only)

Returns the level at the right frequency of the x dB bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Fetch commands

Syntax FETCH:OBwidth:XDBBandwidth:RIGHT:LEVEL?

Related Commands [FETCH:OBWidth:XDBBandwidth:LEFT:LEVEL?](#)

Arguments None

Returns <xdBW_right_level>::=<NRF> is the level at the right frequency in dB.

Examples FETCH:OBWIDTH:XDBBANDWIDTH:RIGHT:LEVEL? might return -23.5, indicating the level at the right frequency is -23.5 dB.

FETCH:PERRor:FERRor? (Query Only)

Returns the frequency error in the Phase error versus Time measurement.

Conditions Measurement views: Phase error versus Time

Group Fetch commands

Syntax FETCH:PERRor:FERRor?

Arguments	None
Returns	<freq_error> ::= <NRf> is the frequency error in Hz.
Examples	FETCh:PERRor:FERRor? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:PERRor:PEAK? (Query Only)

Returns the peak value in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Fetch commands
Syntax	FETCh:PERRor:PEAK?
Related Commands	FETCh:PERRor:PINDeX?
Arguments	None
Returns	<peak> ::= <NRf> is the peak phase error in degrees.
Examples	FETCh:PERRor:PEAK? might return 0.683, indicating the peak phase error is 0.683 °.

FETCh:PERRor:PINDeX? (Query Only)

Returns the time at the phase error peak.

Conditions	Measurement views: Phase error versus Time
Group	Fetch commands
Syntax	FETCh:PERRor:PINDeX?

Related Commands	FETCh:PERRor:PEAK? , [SENSe]:DDEMod:TIME:UNITs
Arguments	None
Returns	<code><peak_time>::=<NRf></code> is the time at the phase error peak in symbol number. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	<code>FETCh:PERRor:PINDEX?</code> might return <code>68.000</code> , indicating that the phase error peak is at symbol #68.

FETCh:PERRor:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Fetch commands
Syntax	<code>FETCh:PERRor:RMS?</code>
Arguments	None
Returns	<code><rms>::=<NRf></code> is the RMS phase error in degrees.
Examples	<code>FETCh:PERRor:RMS?</code> might return <code>0.746</code> , indicating the phase error is 0.746° RMS.

FETCh:PERRor:TRACe? (Query Only)

Returns the Phase error versus Time trace data.

Conditions	Measurement views: Phase error versus Time
Group	Fetch commands

Syntax FETCh:PERRor:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the phase error in degrees at the nth data point,

4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCh:PERRor:TRACe? might return #42036xxxx... (2036-byte data) for the Phase error versus Time trace.

FETCh:PHVTime? (Query Only)

Returns the Phase versus Time trace data.

Conditions Measurement views: Phase versus Time

Group Fetch commands

Syntax FETCh:PHVTime?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the phase in degrees at the nth data point,

4-byte little endian floating-point format specified in IEEE 488.2.

Examples FETCh:PHVTime? might return #3160xxxx... (160-byte data) for the Phase versus Time trace.

FETCh:PHVTime:MAXimum? (Query Only)

Returns the maximum value in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Fetch commands

Syntax FETCh:PHVTime:MAXimum?

Related Commands [FETCh:PHVTime:MAXLocation?](#)

Arguments None

Returns <max> ::= <NRf> is the maximum phase in degrees.

Examples FETCh:PHVTime:MAXimum? might return 153.8, indicating the maximum phase is 153.8 °.

FETCh:PHVTime:MAXLocation? (Query Only)

Returns the time at which the phase is maximum.

Conditions Measurement views: Phase versus Time

Group Fetch commands

Syntax FETCh:PHVTime:MAXLocation?

Related Commands [FETCh:PHVTime:MAXimum?](#)

Arguments None

Returns <max_time> ::= <NRf> is the time in seconds at which the phase is maximum.

Examples `FETCh:PHVTime:MAXLOCATION?` might return `175.3E-9`, indicating the I or Q level is maximum at 175.3 ns.

FETCh:PHVTime:MINimum? (Query Only)

Returns the minimum value in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Fetch commands

Syntax `FETCh:PHVTime:MINimum?`

Related Commands [FETCh:PHVTime:MINLocation?](#)

Arguments None

Returns `<min>::=<Nrf>` is the minimum phase in degrees.

Examples `FETCh:PHVTime:MINIMUM?` might return `-176.3`, indicating the minimum phase is `-176.3 °`.

FETCh:PHVTime:MINLocation? (Query Only)

Returns the time at which the phase is minimum.

Conditions Measurement views: Phase versus Time

Group Fetch commands

Syntax `FETCh:PHVTime:MINLocation?`

Related Commands [FETCh:PHVTime:MINimum?](#)

Arguments None

Returns `<min_time>::=<NRf>` is the time in seconds at which the phase is minimum.

Examples `FETCH:PHVTIME:MINLOCATION?` might return `450.7E-9`, indicating the phase is minimum at 450.7 ns.

FETCH:PHVTime:RESult? (Query Only)

Returns the Phase versus Time measurement results.

Conditions Measurement views: Phase versus Time

Group Fetch commands

Syntax `FETCH:PHVTime:RESult?`

Arguments None

Returns `<max>,<max_time>,<min>,<min_time>`

Where

`<max>::=<NRf>` is the maximum phase in degrees.

`<max_time>::=<NRf>` is the time in seconds at which the phase is maximum.

`<min>::=<NRf>` is the minimum phase in degrees.

`<min_time>::=<NRf>` is the time in seconds at which the phase is minimum.

Examples `FETCH:PHVTIME:RESULT?` might return `153.8,175.3E-9,-176.3,450.7E-9`, indicating the maximum phase is 153.8° at 175.3 ns and the minimum phase is -176.3° at 450.7 ns.

FETCH:PM:PNEGative? (Query Only)

Returns the negative peak phase deviation ($-P_k$) in the PM measurement.

Conditions Measurement views: PM

Group Fetch commands

Syntax `FETCH:PM:PNEGative?`

Arguments	None
Returns	<-Pk> ::= <NRf> is the negative peak phase deviation in degrees.
Examples	FETCh:PM:PNEGATIVE? might return -23.42, indicating the positive peak phase deviation is -23.42 °.

FETCh:PM:PPOSitive? (Query Only)

Returns the positive peak phase deviation (+Pk) in the PM measurement.

Conditions	Measurement views: PM
Group	Fetch commands
Syntax	FETCh:PM:PPOSitive?
Arguments	None
Returns	<+Pk> ::= <NRf> is the positive peak phase deviation in degrees.
Examples	FETCh:PM:PPOSITIVE? might return 26.87, indicating the positive peak phase deviation is 26.87 °.

FETCh:PM:PTPeak? (Query Only)

Returns the peak-peak phase deviation (Pk-Pk) in the PM measurement.

Conditions	Measurement views: PM
Group	Fetch commands
Syntax	FETCh:PM:PTPeak?
Arguments	None

Returns <Pk-Pk> ::= <NRf> is the peak-peak phase deviation in degrees.

Examples FETCH:PM:PTPEAK? might return 46.34, indicating the peak-peak phase deviation is 46.34 °.

FETCH:PM:RESult? (Query Only)

Returns the PM measurement results.

Conditions Measurement views: PM

Group Fetch commands

Syntax FETCH:PM:RESult?

Arguments None

Returns <+Pk>, <-Pk>, <RMS>, <Pk-Pk>

Where

<+Pk> ::= <NRf> is the positive peak phase deviation in degrees.

<-Pk> ::= <NRf> is the negative peak phase deviation in degrees.

<RMS> ::= <NRf> is the RMS phase deviation in degrees.

<Pk-Pk> ::= <NRf> is the peak-peak phase deviation in degrees.

Examples FETCH:PM:RESULT? might return 22.89, -23.45, 15.12, 46.34.

FETCH:PM:RMS? (Query Only)

Returns the RMS phase deviation in the PM measurement.

Conditions Measurement views: PM

Group Fetch commands

Syntax FETCH:PM:RMS?

Arguments	None
Returns	<RMS> ::= <Nrf> is the RMS phase deviation in degrees.
Examples	FETCH:PM:RMS? might return 15.12, indicating the RMS frequency deviation is 15.12 °.

FETCH:PNOise:ALL? (Query Only)

Returns all results of the phase noise measurement.

Conditions	Measurement views: Phase noise
Group	Fetch commands
Syntax	FETCH:PNOise:ALL?
Arguments	None
Returns	<p><Cpower>, <Ferror>, <Pnoise>, <Tjitter>, <Rjitter>, <RFM></p> <p>Where</p> <p><Cpower> ::= <Nrf> is the carrier power in dBm. <Ferror> ::= <Nrf> is the frequency error in Hz. <Pnoise> ::= <Nrf> is the RMS phase noise in degrees. <Tjitter> ::= <Nrf> is the total jitter in seconds. <Rjitter> ::= <Nrf> is the random jitter in seconds. <RFM> ::= <Nrf> is the residual FM in Hz.</p>
Examples	<p>FETCH:PNOISE:ALL? might return -9.455, 1.235E+6, 51.43, 2.312E-9, 4.178E-9, 14.58, indicating Carrier power: -9.455 dBm, Frequency error: 1.235 MHz, RMS phase noise: 51.43 °, Total jitter: 2.312 ns, Random jitter: 4.178 ns, and Residual FM: 14.58 Hz.</p>

FETCh:PNOise:CARRier:FERRor? (Query Only)

Returns the carrier frequency error in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Fetch commands

Syntax FETCh:PNOise:CARRier:FERRor?

Arguments None

Returns <NRf> Carrier frequency error in Hz.

Examples FETCh:PNOISE:CARRIER:FERROR? might return 1.235E+6, indicating that the carrier frequency error is 1.235 MHz.

FETCh:PNOise:CARRier:POWER? (Query Only)

Returns the carrier power in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Fetch commands

Syntax FETCh:PNOise:CARRier:POWER?

Arguments None

Returns <NRf> Carrier power in dBm.
The unit can be changed by the [\[SENSe\]:POWER:UNITs](#) command.

Examples FETCh:PNOISE:CARRIER:POWER? might return -9.455, indicating that the carrier power is -9.455 dBm.

FETCh:PNOise:JITTer? (Query Only)

Returns the jitter in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Fetch commands

Syntax FETCh:PNOise:JITTer?

Arguments None

Returns <NRf> Jitter in seconds.

Examples FETCh:PNOISE:JITTER? might return 2.312E-9, indicating that the jitter is 2.312 ns.

FETCh:PNOise:RESidual:FM? (Query Only)

Returns the residual FM in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Fetch commands

Syntax FETCh:PNOise:RESidual:FM?

Arguments None

Returns <NRf> Residual FM in Hz.

Examples FETCh:PNOISE:RESIDUAL:FM? might return 14.58, indicating that the residual FM is 14.58 Hz.

FETCh:PNOise:RMS:PNOise? (Query Only)

Returns the RMS phase noise in the phase noise measurement.

Conditions	Measurement views: Phase noise
Group	Fetch commands
Syntax	FETCh:PNOise:RMS:PNOise?
Arguments	None
Returns	<NRf> RMS phase noise in degrees.
Examples	FETCh:PNOISE:RMS:PNOISE? might return 51.43, indicating that the RMS phase noise is 51.43 °.

FETCh:PNOise:SPECTrum<x>:X? (Query Only)

Returns the frequencies of the specified trace.

The parameter <x> = 1 and 2, representing Trace 1 and Trace 2, respectively.

Conditions	Measurement views: Phase noise
Group	Fetch commands
Syntax	FETCh:PNOise:SPECTrum<x>:X?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><x(2)>...<x(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)> is the frequency (Hz) at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:PNOISE:SPECTRUM1:X?` might return `#516020xxxx...` (16020-byte data) for the frequencies of Trace 1.

FETCH:PNOise:SPECTrum<x>:XY? (Query Only)

Returns the frequency and phase noise pairs of the specified trace.

The parameter `<x>` = 1 and 2, representing Trace 1 and Trace 2, respectively.

Conditions Measurement views: Phase noise

Group Fetch commands

Syntax `FETCH:PNOise:SPECTrum<x>:XY?`

Arguments None

Returns `#<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)>...<x(n)><y(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<x(n)><y(n)>` is the frequency (Hz) and phase noise (dBc/Hz) pair at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:PNOISE:SPECTRUM1:XY?` might return `#516020xxxx...` (16020-byte data) for the frequency and phase noise pairs of the Trace 1.

FETCH:PNOise:SPECTrum<x>[:Y]? (Query Only)

Returns the phase noise values of the specified trace.

The parameter `<x>` = 1 and 2, representing Trace 1 and Trace 2, respectively.

Conditions Measurement views: Phase noise

Group Fetch commands

Syntax `FETCH:PNOise:SPECTrum<x>[:Y]?`

Arguments	None
Returns	#<num_digit><num_byte><y(1)><y(2)>...<y(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <y(n)> is the phase noise (dBc/Hz) at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	FETCH:PNOISE:SPECTRUM1:Y might return #516020xxxx... (16020-byte data) for the phase noise values of Trace 1.

FETCH:PULSe[:RESult]:ATX? (Query Only)

Returns the average transmitted power in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCH:PULSe[:RESult]:ATX?
Arguments	None
Returns	<first_pulse_num>,<ATX(1)>,< ATX(2)>,...<ATX(n)> Where <first_pulse_num>::=<NR1> is the first pulse number. <ATX(n)>::=<NRf> is the average transmitted power for the pulse with the number of [first_pulse_num + n - 1] in dBm. The unit can be changed to watts by the [SENSe]:POWer:UNITs command. Volt is invalid in the average transmitted power measurement.
Examples	FETCH:PULSE:RESULT:ATX? might return 0,-18.57,-18.73,-18.20,-18.53 for Pulse 0 to 3.

FETCH:PULSe[:RESult]:AVERage? (Query Only)

Returns the average on power in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCh:PULSe[:RESuLt]:AVERAge?
Arguments	None
Returns	<p><first_pulse_num>,< avg(1)>,< avg(2)>,...<avg(n)></p> <p>Where <first_pulse_num>::=<NR1> is the first pulse number. <avg(n)>::=<NRf> is the average on power for the pulse with the number of [first_pulse_num + n - 1] in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.</p>
Examples	FETCh:PULSe:RESuLt:AVERAge? might return 0,-2.354,-2.368,-2.343,-2.358 for Pulse 0 to 3.

FETCh:PULSe[:RESuLt]:DRODb? (Query Only)

Returns the droop in dB in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCh:PULSe[:RESuLt]:DRODb?
Related Commands	FETCh:PULSe[:RESuLt]:DROOp?
Arguments	None
Returns	<p><first_pulse_num>,<droop(1)>,<droop(2)>,...<droop(n)></p> <p>Where <first_pulse_num>::=<NR1> is the first pulse number. <droop(n)>::=<NRf> is the wattage droop for the pulse with the number of [first_pulse_num + n - 1] in dB.</p>

Examples `FETCH:PULSE:RESULT:DRODB?` might return 1, -0.4, 0.32, 0.2, -0.1 for Pulse 1 to 4.

FETCH:PULSe[:RESuLt]:DROOp? (Query Only)

Returns the droop in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESuLt]:DROOp?`

Related Commands [FETCH:PULSe\[:RESuLt\]:DRODb?](#)

Arguments None

Returns `<first_pulse_num>, <droop(1)>, <droop(2)>, ... <droop(n)>`

Where

`<first_pulse_num> ::= <NR1>` is the first pulse number.

`<droop(n)> ::= <NRf>` is the wattage droop for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Examples `FETCH:PULSE:RESULT:DROOP?` might return 0, -270.9E-3, -193.0E-3, -242.7E-3, -177.5E-3 for Pulse 0 to 3.

FETCH:PULSe[:RESuLt]:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESuLt]:DUTPct?`

Arguments	None
Returns	<p><first_pulse_num>, <duty_pct(1)>, <duty_pct(2)>, ... <duty_pct(n)></p> <p>Where <first_pulse_num>::=<NR1> is the first pulse number. <duty_pct(n)>::=<NRf> is the duty factor for the pulse with the number of [first_pulse_num + n - 1] in percent (%).</p>
Examples	<p>FETCH:PULSE:RESULT:DUTPCT? might return 0, 28.94, 28.96, 29.00, 29.01 for Pulse 0 to 3.</p>

FETCH:PULSe[:RESult]:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCH:PULSe[:RESult]:DUTRatio?
Arguments	None
Returns	<p><first_pulse_num>, <duty_ratio(1)>, <duty_ratio(2)>, ... <duty_ratio(n)></p> <p>Where <first_pulse_num>::=<NR1> is the first pulse number. <duty_ratio(n)>::=<NRf> is the duty factor for the pulse with the number of [first_pulse_num + n - 1] (no unit).</p>
Examples	<p>FETCH:PULSE:RESULT:DUTRATIO? might return 0, 289.4E-3, 289.6E-3, 290.0E-3, 290.1E-3 for Pulse 0 to 3.</p>

FETCH:PULSe[:RESult]:FALL? (Query Only)

Returns the fall time in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCH:PULSE[:RESuLt]:FALL?
Arguments	None
Returns	<p><first_pulse_num>, <fall(1)>, <fall(2)>, ... <fall(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <fall(n)> ::= <NRf> is the fall time for the pulse with the number of [first_pulse_num + n - 1] in seconds.</p>
Examples	FETCH:PULSE:RESULT:FALL? might return 0, 110.3E-9, 90.45E-9, 95.03E-9, 111.9E-9 for Pulse 0 to 3.

FETCH:PULSE[:RESuLt]:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCH:PULSE[:RESuLt]:FRDeviation?
Arguments	None
Returns	<p><first_pulse_num>, <freq_dev(1)>, <freq_dev(2)>, ... <freq_dev(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <freq_dev(n)> ::= <NRf> is the frequency deviation for the pulse with the number of [first_pulse_num + n - 1] in Hz.</p>

Examples `FETCH:PULSE:RESULT:FRDEVIATION?` might return 1,740.6E+3, 736.5E+3, 718.3E+3, 672.2E+3 for Pulse 1 to 4.

FETCH:PULSe[:RESuLt]:IRAmplitude? (Query Only)

Returns the pulse impulse response amplitude measurement in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESuLt]:IRAmplitude?`

Arguments None

Returns `<first_pulse_num>, <amplitude(1)>, <amplitude(2)>, ... <amplitude(n)>`

Where

`<first_pulse_num> ::= <NR1>` is the first pulse number.

`<amplitude(n)> ::= <NRf>` is the sidelobe level, in dB, from the mainlobe for the pulse with the number of [`first_pulse_num + n - 1`].

Examples `FETCH:PULSE[:RESULT]:IRAMPLITUDE?` might return 1.0000000000, -45.3, -47.5, -50.2 for Pulse 1 through 3.

FETCH:PULSe[:RESuLt]:IRTime? (Query Only)

Returns the impulse response time in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESuLt]:IRTime?`

Returns `<first_pulse_num>, <time(1)>, <time(2)>, ... <time(n)>`

Where

`<first_pulse_num> ::= <NR1>` is the first pulse number.

`<time(n)> ::= <NRf>` is the sidelobe offset time from the mainlobe for the pulse with the number of `[first_pulse_num + n - 1]` in seconds.

Examples `FETCH:PULSE[:RESULT]:IRTIME?` might return
`1.0000000000,806.6708687693E-9,-846.6595318168E-9,-873.3477443457E-9`
 for Pulse 1 through 3.

FETCH:PULSE[:RESUlt]:MFRReqerror? (Query Only)

Returns the maximum frequency error in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSE[:RESUlt]:MFRReqerror?`

Arguments None

Returns `<first_pulse_num>, <max_freq_err(1)>, <max_freq_err(2)>, ...`
`<max_freq_err(n)>`

Where

`<first_pulse_num> ::= <NR1>` is the first pulse number.

`<max_freq_err(n)> ::= <NRf>` is the maximum frequency error for the pulse with the number of `[first_pulse_num + n - 1]` in Hz.

Examples `FETCH:PULSE:RESULT:MFRREQERROR?` might return
`1,597.5E+3,675.8E+3,642.8E+3,598.2E+3` for Pulse 1 to 4.

FETCH:PULSE[:RESUlt]:MPHerror? (Query Only)

Returns the maximum phase error in the pulse table.

Conditions Measurement views: Pulse table

Group	Fetch commands
Syntax	FETCH:PULSE[:RESULT]:MPHerror?
Arguments	None
Returns	<p><first_pulse_num>, <max_phase_err(1)>, <max_phase_err(2)>, ... <max_phase_err(n)></p> <p>Where <first_pulse_num>::=<NR1> is the first pulse number. <max_phase_err(n)>::=<NRf> is the maximum phase error for the pulse with the number of [first_pulse_num + n - 1] in degrees.</p>
Examples	<p>FETCH:PULSE:RESULT:MPHERROR? might return 1, -9.221, -8.413, -11.853, -10.258 for Pulse 1 to 4.</p>

FETCH:PULSE[:RESULT]:OVEDb? (Query Only)

Returns the overshoot in dB in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCH:PULSE[:RESULT]:OVEDb?
Related Commands	FETCH:PULSE[:RESULT]:OVERshoot?
Arguments	None
Returns	<p><first_pulse_num>, <overshoot(1)>, <overshoot(2)>, ... <overshoot(n)></p> <p>Where <first_pulse_num>::=<NR1> is the first pulse number. <overshoot(n)>::=<NRf> is the overshoot for the pulse with the number of [first_pulse_num + n - 1] in dB.</p>

Examples `FETCH:PULSE:RESULT:OVERDB?` might return `1,1.2,2.3,1.0,0.2` for Pulse 1 to 4.

FETCH:PULSe[:RESUlt]:OVERshoot? (Query Only)

Returns the overshoot in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESUlt]:OVERshoot?`

Related Commands [FETCH:PULSe\[:RESUlt\]:OVEDb?](#)

Arguments None

Returns `<first_pulse_num>, <overshoot(1)>, <overshoot(2)>, ... <overshoot(n)>`

Where

`<first_pulse_num> ::= <NR1>` is the first pulse number.

`<overshoot(n)> ::= <NRf>` is the overshoot for the pulse with the number of `[first_pulse_num + n - 1]` in percent (%) of watts or volts.

Examples `FETCH:PULSE:RESULT:OVERSHOOT?` might return `1,1.2,2.3,1.0,0.2` for Pulse 1 to 4.

FETCH:PULSe[:RESUlt]:PHDeviation? (Query Only)

Returns the phase deviation in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESUlt]:PHDeviation?`

Arguments	None
Returns	<p><first_pulse_num>, <phase_dev(1)>, <phase_dev(2)>, ... <phase_dev(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <phase_dev(n)> ::= <NRf> is the phase deviation for the pulse with the number of [first_pulse_num + n - 1] in degrees.</p>
Examples	<p>FETCH:PULSE:RESULT:PHDEVIATION? might return 1, 11.658, 9.640, 10.509, 8.272 for Pulse 1 to 4.</p>

FETCH:PULSE[:RESuLt]:PPFREquency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCH:PULSE[:RESuLt]:PPFREquency?
Arguments	None
Returns	<p><first_pulse_num>, <pp_freq(1)>, <pp_freq(2)>, ... <pp_freq(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <pp_freq(n)> ::= <NRf> is the pulse-pulse carrier frequency for the pulse with the number of [first_pulse_num + n - 1] in Hz.</p>
Examples	<p>FETCH:PULSE:RESULT:PPFREQUENCY? might return 0, 0.000, 1.258E+3, -3.121E+3, 1.862E+3 for Pulse 0 to 3.</p>

FETCH:PULSE[:RESuLt]:PPOWER? (Query Only)

Returns the peak power in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCh:PULSe[:RESuLt]:PPOWER?
Arguments	None
Returns	<p><first_pulse_num>, <pk_power(1)>, <pk_power(2)>, . . . <pk_power(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <pk_power(n)> ::= <NRf> is the peak power for the pulse with the number of [first_pulse_num + n - 1] in dBm. The unit can be changed by the [SENSe]:POWER:UNITs command.</p>
Examples	FETCh:PULSe:RESuLt:PPOWER? might return 0, -2.26, -2.27, -2.23, -2.25 for Pulse 0 to 3.

FETCh:PULSe[:RESuLt]:PPPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCh:PULSe[:RESuLt]:PPPHase?
Arguments	None
Returns	<p><first_pulse_num>, <pp_phase(1)>, <pp_phase(2)>, . . . <pp_phase(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <pp_phase(n)> ::= <NRf> is the pulse-pulse carrier phase for the pulse with the number of [first_pulse_num + n - 1] in degrees.</p>

Examples `FETCH:PULSE:RESULT:PPHASE?` might return
 0, 0.000, 21.66, 46.76, 57.56 for Pulse 0 to 3.

FETCH:PULSe[:RESuLt]:RINTerval? (Query Only)

Returns the repetition interval in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESuLt]:RINTerval?`

Arguments None

Returns `<first_pulse_num>, <rep_int(1)>, <rep_int(2)>, ... <rep_int(n)>`

Where

`<first_pulse_num>::=<NR1>` is the first pulse number.

`<rep_int(n)>::=<NRf>` is the repetition interval for the pulse with the number of `[first_pulse_num + n - 1]` in seconds.

Examples `FETCH:PULSE:RESULT:RINTERVAL?` might return
 0, 16.03E-6, 16.08E-6, 16.07E-6, 16.02E-6 for Pulse 0 to 3.

FETCH:PULSe[:RESuLt]:RIPDb? (Query Only)

Returns the ripple in dB in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSe[:RESuLt]:RIPDb?`

Related Commands [FETCH:PULSe\[:RESuLt\]:RIPPLE?](#)

Arguments	None
Returns	<code><first_pulse_num></code> , <code><ripple(1)></code> , <code><ripple(2)></code> , ... <code><ripple(n)></code> Where <code><first_pulse_num> ::= <NR1></code> is the first pulse number. <code><ripple(n)> ::= <NRf></code> is the ripple for the pulse with the number of <code>[first_pulse_num + n - 1]</code> in dB.
Examples	<code>FETCH:PULSE:RESULT:RIPDB?</code> might return <code>1,0.4,0.32,0.2,0.1</code> for Pulse 1 to 4.

FETCH:PULSE[:RESULT]:RIPPLE? (Query Only)

Returns the ripple in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	<code>FETCH:PULSE[:RESULT]:RIPPLE?</code>
Related Commands	FETCH:PULSE[:RESULT]:RIPDb?
Arguments	None
Returns	<code><first_pulse_num></code> , <code><ripple(1)></code> , <code><ripple(2)></code> , ... <code><ripple(n)></code> Where <code><first_pulse_num> ::= <NR1></code> is the first pulse number. <code><ripple(n)> ::= <NRf></code> is the volts or watts ripple for the pulse with the number of <code>[first_pulse_num + n - 1]</code> in percent (%).
Examples	<code>FETCH:PULSE:RESULT:RIPPLE?</code> might return <code>0,106.5E-3,177.6E-3,148.3E-3,148.5E-3</code> for Pulse 0 to 3.

FETCH:PULSE[:RESULT]:RISE? (Query Only)

Returns the rise time in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCh:PULSe[:RESuLt]:RISE?
Arguments	None
Returns	<p><first_pulse_num>, <rise(1)>, <rise(2)>, ... <rise(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <rise(n)> ::= <NRf> is the rise time for the pulse with the number of [first_pulse_num + n - 1] in seconds.</p>
Examples	FETCh:PULSE:RESULT:RISE? might return 0, 92.94E-9, 115.9E-9, 115.1E-9, 97.45E-9 for Pulse 0 to 3.

FETCh:PULSe[:RESuLt]:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse table.

Conditions	Measurement views: Pulse table
Group	Fetch commands
Syntax	FETCh:PULSe[:RESuLt]:RMSFreqerror?
Arguments	None
Returns	<p><first_pulse_num>, <RMS_freq_err(1)>, <RMS_freq_err(2)>, ... <RMS_freq_err(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <RMS_freq_err(n)> ::= <NRf> is the RMS frequency error for the pulse with the number of [first_pulse_num + n - 1] in Hz.</p>

Examples `FETCH:PULSE:RESULT:RMSFREQERROR?` might return 1, 51.54E+3, 69.20E+3, 64.21E+3, 51.02E+3 for Pulse 1 to 4.

`FETCH:PULSE[:RESULT]:RMSPherror? (Query Only)`

Returns the RMS phase error in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSE[:RESULT]:RMSPherror?`

Arguments None

Returns `<first_pulse_num>, <RMS_phase_err(1)>, <RMS_phase_err(2)>, ... <RMS_phase_err(n)>`

Where

`<first_pulse_num> ::= <NR1>` is the first pulse number.

`<RMS_phase_err(n)> ::= <NRf>` is the RMS phase error for the pulse with the number of `[first_pulse_num + n - 1]` in degrees.

Examples `FETCH:PULSE:RESULT:RMSPHERROR?` might return 1, 908.4E-3, 752.8E-3, 981.7E-3, 886.4E-3 for Pulse 1 to 4.

`FETCH:PULSE[:RESULT]:RRATE? (Query Only)`

Returns the repetition rate in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax `FETCH:PULSE[:RESULT]:RRATE?`

Arguments None

Returns <first_pulse_num>, <rep_rate(1)>, <rep_rate(2)>, ...
<rep_rate(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<rep_rate(n)>::=<NRf> is the repetition rate for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Examples FETCH:PULSE:RESULT:RRATE? might return 0, 62.50E+3, 62.52E+3, 62.51E+3, 62.49E+3 for Pulse 0 to 3.

FETCH:PULSE[:RESult]:TIME? (Query Only)

Returns the time in the pulse table.

Conditions Measurement views: Pulse table

Group Fetch commands

Syntax FETCH:PULSE[:RESult]:TIME?

Arguments None

Returns <first_pulse_num>, <time(1)>, <time(2)>, ... <time(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<time(n)>::=<NRf> is the time for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Examples FETCH:PULSE:RESULT:TIME? might return 1, 7.937E-3, 8.436E-3, 6.504E-3, 9.876E-3 for Pulse 1 to 4.

FETCH:PULSE[:RESult]:WIDTH? (Query Only)

Returns the pulse width in the pulse table.

Conditions Measurement views: Pulse table

Group	Fetch commands
Syntax	FETCH:PULSE[:RESULT]:WIDTH?
Arguments	None
Returns	<p><first_pulse_num>,<width(1)>,<width(2)>,...<width(n)></p> <p>Where</p> <p><first_pulse_num>::=<NR1> is the first pulse number.</p> <p><width(n)>::=<NRf> is the pulse width for the pulse with the number of [first_pulse_num + n - 1] in seconds.</p>
Examples	<p>FETCH:PULSE:RESULT:WIDTH? might return 0,4.630E-6,4.632E-6,4.639E-6,4.642E-6 for Pulse 0 to 3.</p>

FETCH:PULSE:STATISTICS:ATX? (Query Only)

Returns the average transmitted power in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to TRENd.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCH:PULSE:STATISTICS:ATX?
Arguments	None
Returns	<p><ATX_avg>,<ATX_min>,<ATX_max></p> <p>Where</p> <p><ATX_avg>::=<NRf> is the average of the average transmitted power.</p> <p><ATX_min>::=<NRf> is the minimum of the average transmitted power.</p> <p><ATX_max>::=<NRf> is the maximum of the average transmitted power.</p> <p>Unit: dBm.</p> <p>The unit can be changed to watts by the [SENSE]:POWER:UNITs command.</p> <p>Volt is invalid in the average transmitted power measurement.</p>

Examples `FETCH:PULSE:STATISTICS:ATX?` might return `-18.51,-18.74,-18.12` for the average transmitted power in the pulse statistics.

FETCH:PULSE:STATISTICS:AVERAGE? (Query Only)

Returns the average on power in the pulse statistics. This command is valid when [DISPlay:PULSE:STATISTICS:PLOT](#) is set to TRENd.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSE:STATISTICS:AVERAGE?`

Arguments None

Returns `<avg_avg>,<avg_min>,<avg_max>`

Where

`<avg_avg>::=<NRF>` is the average of the average on power.

`<avg_min>::=<NRF>` is the minimum of the average on power.

`<avg_max>::=<NRF>` is the maximum of the average on power.

Unit: dBm.

The unit can be changed to watts by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `FETCH:PULSE:STATISTICS:AVERAGE?` might return `-2.35,-2.36,-2.34` for the average on power in the pulse statistics.

FETCH:PULSE:STATISTICS:DRODb? (Query Only)

Returns the droop in dB in the pulse statistics. This command is valid when [DISPlay:PULSE:STATISTICS:PLOT](#) is set to TRENd.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSE:STATISTICS:DRODb?`

Related Commands	FETCh:PULSe:STATistics:DROop?
Arguments	None
Returns	<code><droop_avg></code> , <code><droop_min></code> , <code><droop_max></code> Where <code><droop_avg> ::= <NRf></code> is the average droop. <code><droop_min> ::= <NRf></code> is the minimum droop. <code><droop_max> ::= <NRf></code> is the maximum droop. Unit: in dB.
Examples	<code>FETCH:PULSE:STATISTICS:DRODB?</code> might return <code>22.67E-3</code> , <code>-613.5E-3</code> , <code>633.8E-3</code> for the droop in the pulse statistics.

FETCh:PULSe:STATistics:DROop? (Query Only)

Returns the droop in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	<code>FETCh:PULSe:STATistics:DROop?</code>
Related Commands	FETCh:PULSe:STATistics:DRODb?
Arguments	None
Returns	<code><droop_avg></code> , <code><droop_min></code> , <code><droop_max></code> Where <code><droop_avg> ::= <NRf></code> is the average droop. <code><droop_min> ::= <NRf></code> is the minimum droop. <code><droop_max> ::= <NRf></code> is the maximum droop. Unit: Percent (%) by watts.

Examples `FETCH:PULSE:STATISTICS:DROOP?` might return `22.67E-3, -613.5E-3, 633.8E-3` for the droop in the pulse statistics.

FETCH:PULSE:STATISTICS:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse statistics. This command is valid when [DISPlay:PULSE:STATISTICS:PLOT](#) is set to TRENd.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSE:STATISTICS:DUTPct?`

Arguments None

Returns `<duty_pct_avg>, <duty_pct_min>, <duty_pct_max>`

Where

`<duty_pct_avg> ::= <Nrf>` is the average duty factor.

`<duty_pct_min> ::= <Nrf>` is the minimum duty factor.

`<duty_pct_max> ::= <Nrf>` is the maximum duty factor.

Unit: Percent (%).

Examples `FETCH:PULSE:STATISTICS:DUTPCT?` might return `2.437, 2.310, 2.657` for the duty factor (%) in the pulse statistics.

FETCH:PULSE:STATISTICS:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse statistics. This command is valid when [DISPlay:PULSE:STATISTICS:PLOT](#) is set to TRENd.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSE:STATISTICS:DUTRatio?`

Arguments	None
Returns	<code><duty_ratio_avg>,<duty_ratio_min>,<duty_ratio_max></code> Where <code><duty_ratio_avg>::=<NRf></code> is the average duty factor. <code><duty_ratio_min>::=<NRf></code> is the minimum duty factor. <code><duty_ratio_max>::=<NRf></code> is the maximum duty factor. Unit: None.
Examples	<code>FETCH:PULSE:STATISTICS:DUTRATIO?</code> might return <code>24.37E-3,23.11E-3,26.57E-3</code> for the duty factor (ratio) in the pulse statistics.

FETCH:PULSE:STATISTICS:FALL? (Query Only)

Returns the fall time in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	<code>FETCH:PULSE:STATISTICS:FALL?</code>
Arguments	None
Returns	<code><fall_avg>,<fall_min>,<fall_max></code> Where <code><fall_avg>::=<NRf></code> is the average fall time. <code><fall_min>::=<NRf></code> is the minimum fall time. <code><fall_max>::=<NRf></code> is the maximum fall time. Unit: Seconds.
Examples	<code>FETCH:PULSE:STATISTICS:FALL?</code> might return <code>70.27E-9,69.62E-9,71.27E-9</code> for the fall time in the pulse statistics.

FETCh:PULSe:STATistics:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse statistics. This command is valid when `DISPlay:PULSe:STATistics:PLOT` is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCh:PULSe:STATistics:FRDeviation?
Arguments	None
Returns	<code><freq_dev_avg></code> , <code><freq_dev_min></code> , <code><freq_dev_max></code> Where <code><freq_dev_avg> ::= <NRf></code> is the average frequency deviation. <code><freq_dev_min> ::= <NRf></code> is the minimum frequency deviation. <code><freq_dev_max> ::= <NRf></code> is the maximum frequency deviation. Unit: Hz.
Examples	FETCh:PULSe:STATISTICS:FRDEVIATION? might return 754.1E+3, 660.5E+3, 835.2E+3 for the frequency deviation in the pulse statistics.

FETCh:PULSe:STATistics:IRAmplitude? (Query Only)

Returns the Pulse Impulse Response Amplitude measurement in the pulse statistics.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCh:PULSe:STATistics:IRAmplitude?
Arguments	None
Returns	<code><amp_avg></code> , <code><amp_min></code> , <code><amp_max></code>

Where

<amp_avg> ::= <NRf> is the average of the impulse response amplitude.

<amp_min> ::= <NRf> is the minimum of the impulse response amplitude.

<amp_max> ::= <NRf> is the maximum of impulse response amplitude.

Unit: dB.

Examples `FETCH:PULSE:STATISTICS:IRAMPLITUDE?` might return -45.3, -47.1, -43.2 for the impulse response amplitude in the pulse statistics.

FETCH:PULSe:STATistics:IRTime? (Query Only)

Returns the impulse response time in the pulse statistics.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSe:STATistics:IRTime?`

Returns <avg_avg>, <avg_min>, <avg_max>

Where

<avg_avg> ::= <NRf> is the average of the impulse response time.

<avg_min> ::= <NRf> is the minimum of the impulse response time.

<avg_max> ::= <NRf> is the maximum of impulse response time.

Unit: seconds.

Examples `FETCH:PULSE:STATISTICS:IRTIME?` might return -2.35, -2.36, -2.34 for the impulse response time in the pulse statistics.

FETCH:PULSe:STATistics:MFReqerror? (Query Only)

Returns the maximum frequency error in the pulse statistics. This command is valid when `DISPlay:PULSe:STATistics:PLOT` is set to `TREND`.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCh:PULSe:STATistics:MFReqerror?
Arguments	None
Returns	<code><max_freq_err_avg></code> , <code><max_freq_err_min></code> , <code><max_freq_err_max></code> Where <code><max_freq_err_avg>::=<NRf></code> is the average of maximum frequency error. <code><max_freq_err_min>::=<NRf></code> is the minimum of maximum frequency error. <code><max_freq_err_max>::=<NRf></code> is the maximum of maximum frequency error. Unit: Hz.
Examples	FETCh:PULSe:STATISTICS:MFREQERROR? might return 645.0E+3, 555.6E+3, 738.8E+3 for the maximum frequency error in the pulse statistics.

FETCh:PULSe:STATistics:MPHerror? (Query Only)

Returns the maximum phase error in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCh:PULSe:STATistics:MPHerror?
Arguments	None
Returns	<code><max_phase_err_avg></code> , <code><max_phase_err_min></code> , <code><max_phase_err_max></code> Where <code><max_phase_err_avg>::=<NRf></code> is the average of maximum phase error. <code><max_phase_err_min>::=<NRf></code> is the minimum of maximum phase error. <code><max_phase_err_max>::=<NRf></code> is the maximum of maximum phase error.

Unit: Degrees.

Examples `FETCH:PULSE:STATISTICS:MPHERROR?` might return `-11.47,-17.18,-7.61` for the maximum phase error in the pulse statistics.

FETCH:PULSE:STATISTICS:OVEDb? (Query Only)

Returns the overshoot measurement result in dB in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to `TREND` or `TTRend`.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSE:STATISTICS:OVEDb?`

Related Commands [FETCH:PULSE:STATISTICS:OVERshoot?](#)

Arguments None

Returns `<overshoot_avg>,<overshoot_min>,<overshoot_max>`

Where

`<overshoot_avg>::=<NRf>` is the average overshoot.

`<overshoot_min>::=<NRf>` is the minimum overshoot.

`<overshoot_max>::=<NRf>` is the maximum overshoot.

Unit: dB.

Examples `FETCH:PULSE:STATISTICS:OVEDB?` might return `0.3,0.1,0.5` for the overshoot measurement result in dB in the pulse statistics.

FETCH:PULSE:STATISTICS:OVERshoot? (Query Only)

Returns the overshoot in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to `TREND` or `TTRend`.

Conditions Measurement views: Pulse statistics

Group	Fetch commands
Syntax	FETCH:PULSE:STATISTICS:OVERSHOOT?
Related Commands	FETCh:PULSe:STATistics:OVEDb?
Arguments	None
Returns	<p><overshoot_avg>, <overshoot_min>, <overshoot_max></p> <p>Where</p> <p><overshoot_avg> ::= <NRf> is the average overshoot.</p> <p><overshoot_min> ::= <NRf> is the minimum overshoot.</p> <p><overshoot_max> ::= <NRf> is the maximum overshoot.</p> <p>Unit: Percent (%) by watts or volts.</p>
Examples	<p>FETCH:PULSE:STATISTICS:OVERSHOOT? might return 0.3,0.1,0.5 for the overshoot in the pulse statistics.</p>

FETCh:PULSe:STATistics:PHDeviation? (Query Only)

Returns the phase deviation in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCh:PULSe:STATistics:PHDeviation?
Arguments	None
Returns	<p><phase_dev_avg>, <phase_dev_min>, <phase_dev_max></p> <p>Where</p> <p><phase_dev_avg> ::= <NRf> is the average phase deviation.</p> <p><phase_dev_min> ::= <NRf> is the minimum phase deviation.</p> <p><phase_dev_max> ::= <NRf> is the maximum phase deviation.</p> <p>Unit: Degrees.</p>

Examples `FETCH:PULSE:STATISTICS:PHDEVIATION?` might return 11.678, 7.694, 17.374 for the phase deviation in the pulse statistics.

FETCH:PULSe:STATistics:PPFrequency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse statistics. This command is valid when `DISPlay:PULSe:STATistics:PLOT` is set to TREND.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSe:STATistics:PPFrequency?`

Arguments None

Returns `<pp_freq_avg>, <pp_freq_min>, <pp_freq_max>`

Where

`<pp_freq_avg>::=<NRf>` is the average pulse-pulse carrier frequency.

`<pp_freq_min>::=<NRf>` is the minimum pulse-pulse carrier frequency.

`<pp_freq_max>::=<NRf>` is the maximum pulse-pulse carrier frequency.

Unit: Hz.

Examples `FETCH:PULSE:STATISTICS:PPFREQUENCY?` might return 1.135E+3, 311.3E+3, -262.8E+3 for the pulse-pulse carrier frequency in the pulse statistics.

FETCH:PULSe:STATistics:PPOWer? (Query Only)

Returns the peak power in the pulse statistics. This command is valid when `DISPlay:PULSe:STATistics:PLOT` is set to TREND.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSe:STATistics:PPOWer?`

Arguments	None
Returns	<code><pk_power_avg></code> , <code><pk_power_min></code> , <code><pk_power_max></code> Where <code><pk_power_avg></code> ::= <code><NRf></code> is the average peak power. <code><pk_power_min></code> ::= <code><NRf></code> is the minimum peak power. <code><pk_power_max></code> ::= <code><NRf></code> is the maximum peak power. Unit: dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	<code>FETCH:PULSE:STATISTICS:PPOWER?</code> might return <code>-2.273</code> , <code>-2.313</code> , <code>-2.235</code> for the peak power in the pulse statistics.

FETCH:PULSe:STATistics:PPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	<code>FETCH:PULSe:STATistics:PPHase?</code>
Arguments	None
Returns	<code><pp_phase_avg></code> , <code><pp_phase_min></code> , <code><pp_phase_max></code> Where <code><pp_phase_avg></code> ::= <code><NRf></code> is the average pulse-pulse carrier phase. <code><pp_phase_min></code> ::= <code><NRf></code> is the minimum pulse-pulse carrier phase. <code><pp_phase_max></code> ::= <code><NRf></code> is the maximum pulse-pulse carrier phase. Unit: Degrees.
Examples	<code>FETCH:PULSE:STATISTICS:PPHASE?</code> might return <code>-9.298E-3</code> , <code>-254.3E-3</code> , <code>311.7E-3</code> for the pulse-pulse carrier phase in the pulse statistics.

FETCH:PULSE:STATISTICS:RINTERVAL? (Query Only)

Returns the repetition interval in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax FETCH:PULSE:STATISTICS:RINTERVAL?

Arguments None

Returns <rep_int_avg>,<rep_int_min>,<rep_int_max>

Where

<rep_int_avg>::=<NRf> is the average repetition interval.

<rep_int_min>::=<NRf> is the minimum repetition interval.

<rep_int_max>::=<NRf> is the maximum repetition interval.

Unit: Seconds.

Examples FETCH:PULSE:STATISTICS:RINTERVAL? might return 240.5E-6,217.9E-6,281.2E-6 for the repetition interval in the pulse statistics.

FETCH:PULSE:STATISTICS:RIPDB? (Query Only)

Returns the ripple in dB in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax FETCH:PULSE:STATISTICS:RIPDB?

Related Commands [FETCH:PULSE:STATISTICS:RIPPLE?](#)

Arguments None

Returns <ripple_avg>, <ripple_min>, <ripple_max>

Where

<ripple_avg>::=<NRf> is the average ripple.

<ripple_min>::=<NRf> is the minimum ripple.

<ripple_max>::=<NRf> is the maximum ripple.

Unit: dB.

Examples FETCH:PULSE:STATISTICS:RIPDB? might return
160.4E-3, 83.78E-3, 287.7E-3 for the ripple in dB in the pulse statistics.

FETCH:PULSE:STATISTICS:RIPPLE? (Query Only)

Returns the ripple in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax FETCH:PULSE:STATISTICS:RIPPLE?

Related Commands [FETCH:PULSE:STATISTICS:RIPDB?](#)

Arguments None

Returns <ripple_avg>, <ripple_min>, <ripple_max>

Where

<ripple_avg>::=<NRf> is the average ripple.

<ripple_min>::=<NRf> is the minimum ripple.

<ripple_max>::=<NRf> is the maximum ripple.

Unit: Percent (%) by watts or volts.

Examples FETCH:PULSE:STATISTICS:RIPPLE? might return
160.4E-3, 83.78E-3, 287.7E-3 for the ripple in the pulse statistics.

FETCh:PULSe:STATistics:RISE? (Query Only)

Returns the rise time in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCh:PULSe:STATistics:RISE?
Arguments	None
Returns	<code><rise_avg></code> , <code><rise_min></code> , <code><rise_max></code> Where <code><rise_avg> ::= <NRf></code> is the average rise time. <code><rise_min> ::= <NRf></code> is the minimum rise time. <code><rise_max> ::= <NRf></code> is the maximum rise time. Unit: Seconds.
Examples	FETCh:PULSe:STATISTICS:RISE? might return 105.4E-9, 91.65E-9, 116.2E-9 for the rise time in the pulse statistics.

FETCh:PULSe:STATistics:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCh:PULSe:STATistics:RMSFreqerror?
Arguments	None
Returns	<code><RMS_freq_err_avg></code> , <code><RMS_freq_err_min></code> , <code><RMS_freq_err_max></code>

Where

<RMS_freq_err_avg>::=<Nrf> is the average of RMS frequency error.

<RMS_freq_err_min>::=<Nrf> is the minimum of RMS frequency error.

<RMS_freq_err_max>::=<Nrf> is the maximum of RMS frequency error.

Unit: Hz.

Examples `FETCH:PULSE:STATISTICS:RMSFREQERROR?` might return 63.67E+3, 45.49E+3, 81.28E+3 for the RMS frequency error in the pulse statistics.

FETCH:PULSe:STATistics:RMSPherror? (Query Only)

Returns the RMS phase error in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSe:STATistics:RMSPherror?`

Arguments None

Returns <RMS_phase_err_avg>, <RMS_phase_err_min>, <RMS_phase_err_max>

Where

<RMS_phase_err_avg>::=<Nrf> is the average of RMS phase error.

<RMS_phase_err_min>::=<Nrf> is the minimum of RMS phase error.

<RMS_phase_err_max>::=<Nrf> is the maximum of RMS phase error.

Unit: Degrees.

Examples `FETCH:PULSE:STATISTICS:RMSPHERROR?` might return 1.032, 604.5E-3, 1.606 for the RMS phase error in the pulse statistics.

FETCH:PULSe:STATistics:RRATE? (Query Only)

Returns the repetition rate in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse trace

Group	Fetch commands
Syntax	<code>FETCh:PULSe:STATistics:RRATE?</code>
Arguments	None
Returns	<code><rep_rate_avg></code> , <code><rep_rate_min></code> , <code><rep_rate_max></code> Where <code><rep_rate_avg> ::= <NRf></code> is the average repetition rate. <code><rep_rate_min> ::= <NRf></code> is the minimum repetition rate. <code><rep_rate_max> ::= <NRf></code> is the maximum repetition rate. Unit: Hz.
Examples	<code>FETCh:PULSe:STATISTICS:RRATE?</code> might return <code>62.50E+3</code> , <code>62.49E+3</code> , <code>62.52E+3</code> for the repetition rate in the pulse statistics.

FETCh:PULSe:STATistics:WIDTh? (Query Only)

Returns the pulse width in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse trace
Group	Fetch commands
Syntax	<code>FETCh:PULSe:STATistics:WIDTh?</code>
Arguments	None
Returns	<code><width_avg></code> , <code><width_min></code> , <code><width_max></code> Where <code><width_avg> ::= <NRf></code> is the average pulse width. <code><width_min> ::= <NRf></code> is the minimum pulse width. <code><width_max> ::= <NRf></code> is the maximum pulse width. Unit: Seconds.

Examples `FETCH:PULSE:STATISTICS:WIDTH?` might return 4.636E-6, 4.630E-6, 4.643E-6 for the pulse width in the pulse statistics.

FETCH:PULSe:STATistics:X? (Query Only)

Returns the horizontal values of the trace data of the pulse statistics measurement selected by the `DISPlay:PULSe:SElect:RESult` command.

NOTE. Select the plot type (Trend, FFT, Time Trend or Histogram) using the `DISPlay:PULSe:STATistics:PLOT` command before executing this query.

Conditions Measurement views: Pulse statistics

Group Fetch commands

Syntax `FETCH:PULSe:STATistics:X?`

Arguments None

Returns `#<num_digit><num_byte><data1><data2>...data<n>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the horizontal value of the statistics graph at the n^{th} data point.

The unit is trace number (Plot = Trend), Hz (Plot = FFT), second (Plot = Time Trend) or current measurement unit (Plot = Histogram).

4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:PULSE:STATISTICS:X?` might return `#264xxxx...` (64-byte data) for the statistics trace of the pulse width measurement when `DISPlay:PULSe:SElect:RESult` is set to `WIDTH`.

FETCH:PULSe:STATistics:XY? (Query Only)

Returns the horizontal and vertical values of the trace data of the pulse statistics measurement selected by the `DISPlay:PULSe:SElect:RESult` command.

NOTE. Select the plot type (Trend, FFT, Time Trend or Histogram) using the *DISPlay:PULSe:STATistics:PLOT* command before executing this query.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	FETCH:PULSE:STATISTICS:XY?
Arguments	None
Returns	<p>#<num_digit><num_byte><data1><data2>...data<n></p> <p>Where</p> <p><num_digit> is the number of digits in <num_byte>.</p> <p><num_byte> is the number of bytes of data that follow.</p> <p><data(n)> is the horizontal value of the statistics graph at the nth data point.</p> <p><data(n+1)> is the vertical value of the statistics graph at the nth data point.</p> <p>For horizontal values, the unit is trace number (Plot = Trend), Hz (Plot = FFT), second (Plot = Time Trend) or current measurement unit (Plot = Histogram).</p> <p>For vertical values, the unit is current measurement unit (Plot = Trend or Time Trend), dB (Plot = FFT), count (Plot = Histogram)</p> <p>4-byte little endian floating-point format specified in IEEE 488.2.</p>
Examples	<p>FETCH:PULSE:STATISTICS:XY? might return #264xxxx... (64-byte data) for the statistics trace of the pulse width measurement when DISPlay:PULSe:SElect:RESult is set to WIDTHh.</p>

FETCH:PULSe:STATistics[:Y]? (Query Only)

Returns the trace data of the pulse statistics measurement selected by the *DISPlay:PULSe:SElect:RESult* command.

NOTE. Select the plot type (Trend, FFT, Time Trend or Histogram) using the *DISPlay:PULSe:STATistics:PLOT* command before executing this query.

Conditions	Measurement views: Pulse statistics
-------------------	-------------------------------------

Group	Fetch commands
Syntax	FETCh:PULSe:STATISTICS[:Y]?
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude at the n th data point. The unit is current measurement unit (Plot = Trend or Time Trend), dB (Plot = FFT), count or percent (Plot = Histogram) 4-byte little endian floating-point format specified in IEEE 488.2. The unit of power is selected by the [SENSe]:POWer:UNITs command.
Examples	FETCh:PULSe:STATISTICS[:Y]? might return #264xxxx... (64-byte data) for the statistics trace of the pulse width measurement when DISPlay:PULSe:SElect:RESult is set to WIDTH.

FETCh:PULSe:TRACe:X? (Query Only)

Returns the time values of the pulse trace. Use the [DISPlay:PULSe:SElect:NUMBer](#) command to select the pulse, and the [DISPlay:PULSe:SElect:RESult](#) command to select the measurement result.

Conditions	Measurement views: Pulse trace
Group	Fetch commands
Syntax	FETCh:PULSe:TRACe:X?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><x(2)>...<x(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)> is the time in seconds at the n th data point,

4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:PULSE:TRACE:X?` might return `#43204xxxx...` (3204-byte data) for the time values of the trace.

FETCh:PULSe:TRACe:XY? (Query Only)

Returns the horizontal (time) and vertical value pairs of the pulse trace. Use the [DISPlay:PULSe:SElect:NUMBer](#) command to select the pulse, and the [DISPlay:PULSe:SElect:RESult](#) command to select the measurement result.

Conditions Measurement views: Pulse trace

Group Fetch commands

Syntax `FETCh:PULSe:TRACe:XY?`

Arguments None

Returns `#<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)>...<x(n)><y(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<x(n)><y(n)>` is the horizontal value (time in seconds) and vertical value pair at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2.

The vertical unit depends on measurement results: Hz for frequency error and deviation, degrees for phase error and deviation, otherwise dBm. The vertical unit can be changed by the [\[SENSE\]:POWER:UNITs](#) command.

Examples `FETCH:PULSE:TRACE:XY?` might return `#43204xxxx...` (3204-byte data) for the horizontal (time) and vertical value pairs of the pulse trace.

FETCh:PULSe:TRACe[:Y]? (Query Only)

Returns the vertical values of the pulse trace. Use the [DISPlay:PULSe:SElect:NUMBer](#) command to select the pulse, and the [DISPlay:PULSe:SElect:RESult](#) command to select the measurement result.

Conditions	Measurement views: Pulse trace
Group	Fetch commands
Syntax	<code>FETCh:PULSe:TRACe[:Y]?</code>
Arguments	None
Returns	<code>#<num_digit><num_byte><y(1)><y(2)>...<y(n)></code> Where <code><num_digit></code> is the number of digits in <code><num_byte></code> . <code><num_byte></code> is the number of bytes of data that follow. <code><y(n)></code> is the amplitude (dBm) at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2. The unit depends on measurement results: Hz for frequency error and deviation, degrees for phase error and deviation, otherwise dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	<code>FETCh:PULSe:TRACe:Y?</code> might return <code>#43204xxxx...</code> (3204-byte data) for the vertical values of the pulse trace.

FETCh:RFIN:IQ? (Query Only)

Returns time-domain IQ data for a specific acquisition data record. You can set a range of IQ pairs optionally. The instrument needs to be in stopped mode. If not in stopped mode, it returns the execution error (-200).

Conditions	Measurement views: All
Group	Fetch commands
Syntax	<code>FETCh:RFIN:IQ? <rec_ID>[, <begin_num>, <end_num>]</code>
Arguments	<code><rec_ID></code> specifies the acquisition data record ID number. <code><begin_num></code> specifies the beginning number of IQ pairs. <code><end_num></code> specifies the end number of IQ pairs. Use the FETCh:RFIN:RECOrd:IDS? query to get the beginning and end ID's of acquisition data records.

Returns #<num_digit><num_byte><I(1)><Q(1)><I(2)><Q(2)>...<I(n)><Q(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<I(n)> and <Q(n)> are the time-domain IQ data pair.

4-byte little endian floating-point format specified in IEEE 488.2.

To find out the range of IQ pairs, use the [FETCh:RFIN:IQ:HEADer?](#) query. The returned value of <num_sample> is the number of IQ pairs.

NOTE. *Do not fetch a large number of IQ pairs because of memory limitation.*

Examples FETCh:RFIN:IQ? 10,25,350 might return #43848xxxx... (3848-byte data) for the record #10, ranging from 25th to 350th IQ pair.

FETCh:RFIN:IQ:HEADer? (Query Only)

Returns the header information for a specific acquisition data record. The instrument needs to be in stopped mode. If not in stopped mode, it returns the execution error (-200).

Conditions Measurement views: All

Group Fetch commands

Syntax FETCh:RFIN:IQ:HEADer? <rec_ID>

Arguments <rec_ID> specifies the acquisition data record ID number.

Use the [FETCh:RFIN:RECORD:IDS?](#) query to get the beginning and end ID's of acquisition data records.

Returns ,<sampling_freq>,<num_sample>,<center_freq>,<acq_BW>,<ref_level>,<trig_pos>,<time_stamp>,<FastFrame_ID>

Where

 ::= <NR3> is the span in Hz.

<sampling_freq> ::= <NR3> is the sampling frequency in Hz.

<num_sample> ::= <NR3> is the number of samples.

<center_freq> ::= <NR3> is the center frequency in Hz.

<acq_BW> ::= <NR3> is the acquisition bandwidth in Hz.

<ref_level> ::= <NR3> is the reference level in dBm.

<trig_pos>::=<NR3> is the trigger position in seconds.
 <time_stamp>::=<string> is the time stamp.
 <FastFrame_ID>::=<NR1> is the Fast Frame ID: Zero or positive number.
 If the Fast Frame is disabled, the ID will be negative.

Examples FETCH:RFIN:IQ:HEADER? 10 might return 40.0E+6, 50.0E+6, 4.027E+3, 1.5E+9, 40.0E+6, 0.0, 20.242E-6, "10/31/2007 1118:32 AM", -1, indicating
 Span: 40 MHz,
 Sampling frequency: 50 MHz,
 Number of samples: 4027,
 Center frequency: 1.5 GHz,
 Acquisition bandwidth: 40 MHz,
 Reference level: 0 dBm,
 Trigger position: 20.242 μ s,
 Time stamp: 10/31/2007 1118:32 AM, and
 Fast Frame ID: -1

FETCh:RFIN:IQ:SCALe? (Query Only)

Returns the internal RF linear data scaling factor contained in the .tiq file header. The scaling factor can be used to convert digital IQ output (Option 05) values into real IQ values.

Conditions Measurement views: All

Group Fetch commands

Syntax FETCh:RFIN:IQ:SCALe?

Related Commands [FETCh:RFIN:RECOrd:IDS?](#)

Arguments None

Returns <NR3> The RF linear data scaling factor.

Examples FETCH:RFIN:IQ:SCALE? might return 19.553E-6 for the scaling factor.

FETCh:RFIN:RECOrd:IDS? (Query Only)

Returns the beginning and end ID numbers of acquisition data.

NOTE. *The instrument needs to be in stopped mode. If not in stopped mode, it returns the execution error (-200).*

Conditions Measurement views: All

Group Fetch commands

Syntax FETCh:RFIN:RECOrd:IDS?

Arguments None

Returns <begin_ID>, <end_ID>

Where

<begin_ID> ::= <NR1> is the beginning ID of acquisition data.

<end_ID> ::= <NR1> is the end ID of acquisition data.

NOTE. *“-1,-1” is returned when the span changes and the acquisition is armed, but the acquisition has not yet occurred.*

Examples FETCh:RFIN:RECOrd:IDS? might return 1, 147, indicating the beginning and end ID's of acquisition data are 1 and 147, respectively.

FETCh:SGRam? (Query Only)

Returns trace data of a line in the spectrogram. The line is selected using the [TRACe:SGRam:SELEct:LINE](#) command.

Conditions Measurement views: Spectrogram

Group Fetch commands

Syntax FETCh:SGRam?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where
 <num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <data(n)> is the amplitude in dBm at the nth data point,
 4-byte little endian floating-point format specified in IEEE 488.2.
 The unit can be changed by the [SENSE]:POWER:UNITS command.

Examples FETCH:SGRAM? might return #43204xxxx... (3204-byte data) for the line in the spectrogram.

FETCH:SPECTrum:TRACe<x>? (Query Only)

Returns the trace data in the Spectrum measurement.

The parameter <x> = 1 to 5.

NOTE. TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.

Conditions Measurement views: Spectrum

Group Fetch commands

Syntax FETCH:SPECTrum:TRACe<x>?

Related Commands TRACe<x>:SPECTrum command subgroup

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where
 <num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <data(n)> is the amplitude in dBm at the nth data point,
 4-byte little endian floating-point format specified in IEEE 488.2.
 The unit can be changed by the [SENSE]:POWER:UNITS command.

Examples `FETCH:SPECTRUM:TRACE1?` might return `#43204xxxx...` (3204-byte data) for Trace 1 in the Spectrum measurement.

FETCH:SPURious:CARRier:POWer? (Query Only)

Returns the carrier power in the Spurious measurement.

Conditions Measurement views: Spurious

Group Fetch commands

Syntax `FETCH:SPURious:CARRier:POWer?`

Arguments None

Returns `<Nrf>` Carrier power in dBm.
The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `FETCH:SPURIOUS:CARRIER:POWER?` might return `4.227`, indicating that the carrier power is 4.227 dBm.

FETCH:SPURious:COUNT? (Query Only)

Returns the number of spurious signals in the Spurious measurement.

Conditions Measurement views: Spurious

Group Fetch commands

Syntax `FETCH:SPURious:COUNT?`

Arguments None

Returns `<Nrf>` The number of spurious signals.

Examples `FETCH:SPURIOUS:COUNT?` might return `4`, indicating that the spurious count is 4.

FETCh:SPURious:PASS? (Query Only)

Returns the pass/fail limit test result in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Fetch commands
Syntax	FETCh:SPURious:PASS?
Arguments	None
Returns	0 (fail) or 1 (pass).
Examples	FETCh:SPURIOUS:PASS? might return 1, indicating that the limit test was successful.

FETCh:SPURious:SPECTrum:X? (Query Only)

Returns the frequencies of the spectrum trace in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Fetch commands
Syntax	FETCh:SPURious:SPECTrum:X?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><x(2)>...<x(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)> is the frequency (Hz) at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `FETCH:SPURIOUS:SPECTRUM:X?` might return `#516020xxxx...` (16020-byte data) for the frequencies of the spectrum trace in the Spurious measurement.

FETCH:SPURious:SPECTrum:XY? (Query Only)

Returns the frequency and amplitude pairs of the spectrum trace in the Spurious measurement.

Conditions Measurement views: Spurious

Group Fetch commands

Syntax `FETCH:SPURious:SPECTrum:XY?`

Arguments None

Returns `#<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)>...<x(n)><y(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<x(n)><y(n)>` is the frequency (Hz) and amplitude (dBm) pair at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2.

The amplitude unit can be changed by the [\[SENSE\]:POWER:UNITS](#) command.

Examples `FETCH:SPURIOUS:SPECTRUM:XY?` might return `#516020xxxx...` (16020-byte data) for the frequency and amplitude pairs of the spectrum trace in the Spurious measurement.

FETCH:SPURious:SPECTrum[:Y]? (Query Only)

Returns the amplitudes of the spectrum trace in the Spurious measurement.

Conditions Measurement views: Spurious

Group Fetch commands

Syntax `FETCH:SPURious:SPECTrum[:Y]?`

Arguments	None
Returns	<code>#<num_digit><num_byte><y(1)><y(2)>...<y(n)></code> Where <code><num_digit></code> is the number of digits in <code><num_byte></code> . <code><num_byte></code> is the number of bytes of data that follow. <code><y(n)></code> is the amplitude (dBm) at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2. The unit can be changed by the <code>[SENSE]:POWER:UNITs</code> command.
Examples	<code>FETCH:SPURIOUS:SPECTRUM:Y?</code> might return <code>#516020xxxx...</code> (16020-byte data) for the amplitudes of the spectrum trace in the Spurious measurement.

FETCH:SPURious:SPUR<x>:AMPLitude:ABSolute? (Query Only)

Returns the absolute amplitude of the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Fetch commands
Syntax	<code>FETCH:SPURious:SPUR<x>:AMPLitude:ABSolute?</code>
Arguments	None
Returns	<code><NRF></code> Absolute amplitude of the specified spurious signal in dBm. The unit can be changed by the <code>[SENSE]:POWER:UNITs</code> command.
Examples	<code>FETCH:SPURIOUS:SPUR1:AMPLITUDE:ABSOLUTE?</code> might return <code>-19.782</code> , indicating that the absolute amplitude of Spurious #1 is -19.782 dBm.

FETCH:SPURious:SPUR<x>:AMPLitude:RELative? (Query Only)

Returns the relative amplitude of the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
-------------------	-----------------------------

Group	Fetch commands
Syntax	<code>FETCh:SPURious:SPUR<x>:AMPLitude:RELative?</code>
Arguments	None
Returns	<NRf> Relative amplitude of the specified spurious signal in dB. Use the [SENSe]:SPURious:REFerence command to set the power reference.
Examples	<code>FETCh:SPURIOUS:SPUR1:AMPLITUDE:RELATIVE?</code> might return <code>-9.782</code> , indicating that the relative amplitude of Spurious #1 is -9.782 dB.

FETCh:SPURious:SPUR<x>:FREQuency:ABSolute? (Query Only)

Returns the absolute frequency of the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Fetch commands
Syntax	<code>FETCh:SPURious:SPUR<x>:FREQuency:ABSolute?</code>
Arguments	None
Returns	<NRf> Absolute frequency of the spurious signal in Hz.
Examples	<code>FETCh:SPURIOUS:SPUR1:FREQUENCY:ABSOLUTE?</code> might return <code>2.235E+9</code> , indicating that the absolute frequency of Spurious #1 is 2.235 GHz.

FETCh:SPURious:SPUR<x>:FREQuency:RELative? (Query Only)

Returns the relative frequency of the specified spurious signal to the carrier in the Spurious measurement. This command is valid when [\[SENSe\]:SPURious:REFerence](#) is set to `CARRier`.

Conditions	Measurement views: Spurious
-------------------	-----------------------------

Group	Fetch commands
Syntax	FETCh:SPURious:SPUR<x>:FREQUency:RELative?
Arguments	None
Returns	<NRF> Relative frequency of the spurious signal to the carrier in Hz.
Examples	FETCh:SPURIOUS:SPUR1:FREQUENCY:RELATIVE might return 3.634E+6, indicating that the relative frequency of Spurious #1 is 3.634 MHz.

FETCh:SPURious:SPUR<x>:LIMit:ABSolute? (Query Only)

Returns the absolute amplitude of the limit for the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Fetch commands
Syntax	FETCh:SPURious:SPUR<x>:LIMit:ABSolute?
Arguments	None
Returns	<NRF> Absolute amplitude of the limit for the specified spurious signal in dBm. The unit can be changed by the [SENSE]:POWER:UNITs command.
Examples	FETCh:SPURIOUS:SPUR1:LIMIT:ABSOLUTE? might return -50.0, indicating that the absolute amplitude of the limit for Spurious #1 is -50 dBm.

FETCh:SPURious:SPUR<x>:LIMit:RELative? (Query Only)

Returns the relative amplitude of the limit for the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
-------------------	-----------------------------

Group	Fetch commands
Syntax	FETCh:SPURious:SPUR<x>:LIMit:RELative?
Arguments	None
Returns	<NRF> Relative amplitude of the limit for the specified spurious signal in dB. Use the [SENSe]:SPURious:REFerence command to set the power reference.
Examples	FETCh:SPURIOUS:SPUR1:LIMIT:RELATIVE? might return -10.0, indicating that the relative amplitude of the limit for Spurious #1 is -10 dB.

FETCh:SPURious:SPUR<x>:LIMit:VIOLation? (Query Only)

Returns whether the specified spurious signal exceeds the limit or not.

Conditions	Measurement views: Spurious
Group	Fetch commands
Syntax	FETCh:SPURious:SPUR<x>:LIMit:VIOLation?
Arguments	None
Returns	0 (under the limit) or 1 (over the limit).
Examples	FETCh:SPURIOUS:SPUR1:LIMIT:VIOLATION? might return 1, indicating that Spurious #1 exceeds the limit.

FETCh:SPURious:SPUR<x>:RANGe? (Query Only)

Returns the frequency range in which the specified spurious signal occurred.

Conditions	Measurement views: Spurious
Group	Fetch commands

Syntax	<code>FETCh:SPURious:SPUR<x>:RANGE?</code>
Arguments	None
Returns	<string> "A" to "T" representing Range A to T, respectively.
Examples	<code>FETCh:SPURIOUS:SPUR1:RANGE</code> might return "E", indicating that Spurious #1 is in Range E.

FETCh:SQUality:FREQuency:DEVIation? (Query Only)

Returns the frequency deviation in the signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to C4FM, FSK2, FSK4, FSK8, or FSK16.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	<code>FETCh:SQUality:FREQuency:DEVIation?</code>
Arguments	None
Returns	<NRF> Frequency deviation in Hz.
Examples	<code>FETCh:SQUALITY:FREQUENCY:DEVIATION?</code> might return <code>12.68E+3</code> , indicating the frequency deviation is 12.68 kHz.

FETCh:SQUality:FREQuency:DEVIation:TABLE? (Query Only)

Returns the number of columns and the values in the frequency deviation table for a signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to C4FM, FSK2, FSK4, FSK8, or FSK16.

Conditions	Measurement views: Signal quality
-------------------	-----------------------------------

Group	Fetch commands
Syntax	FETCH:SQUALITY:FREQUENCY:DEVIATION:TABLE?
Arguments	None
Returns	<p><Dev_Num>, {<Freq_dev_Max>, <Freq_dev_Min>, <Freq_dev_Avg>}</p> <p>Where</p> <p><Dev_Num> ::= <NR1> is the number of columns in the frequency deviation table. = 2 (2FSK), 4 (4FSK, C4FM), 8 (8FSK), or 16 (16FSK)</p> <p><Freq_dev_Max> ::= <NRf> is the maximum frequency deviation in Hz.</p> <p><Freq_dev_Min> ::= <NRf> is the minimum frequency deviation in Hz.</p> <p><Freq_dev_Avg> ::= <NRf> is the average frequency deviation in Hz.</p> <p>The dataset <Freq_dev_Max>, <Freq_dev_Min>, <Freq_dev_Avg> is returned for each symbol in ascending order of its level (for example, in order of symbol -3, -1, +1, and +3 for 4FSK).</p>
Examples	<p>FETCH:SQUALITY:FREQUENCY:DEVIATION:TABLE? might return 2, 1.257E+3, 1.039E+3, 1.162E+3, 1.586E+3, 1.298E+3, 1.425E+3 for the frequency signal, populating the results table as follows.</p>

Deviations	-1	+1
Maximum	1.257 kHz	1.586 kHz
Minimum	1.039 kHz	1.298 kHz
Average	1.162 kHz	1.425 kHz

FETCH:SQUALITY:FREQUENCY:ERROR? (Query Only)

Returns the frequency error in the signal quality measurement.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	FETCH:SQUALITY:FREQUENCY:ERROR?
Arguments	None

Returns <NRf> Frequency error in Hz.

Examples FETCH:SQUALITY:FREQUENCY:ERROR? might return 612.043E+3, indicating that the frequency error is 612.043 kHz.

FETCh:SQUality:GAIN:IMBalance? (Query Only)

Returns the gain imbalance in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax FETCh:SQUality:GAIN:IMBalance?

Arguments None

Returns <NRf> Gain imbalance in dB.

Examples FETCH:SQUALITY:GAIN:IMBALANCE? might return -57.746E-3, indicating that the gain imbalance is -0.057746 dB.

FETCh:SQUality:ORIGin:OFFSet? (Query Only)

Returns the origin offset in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax FETCh:SQUality:ORIGin:OFFSet?

Arguments None

Returns <NRf> Origin offset in dB.

Examples `FETCH:SQUALITY:ORIGIN:OFFSET?` might return `-44.968`, indicating that the origin offset is `-44.968` dB.

FETCH:SQUALITY:PEAK:EVM? (Query Only)

Returns the peak EVM (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:EVM?`

Arguments None

Returns `<NRf>` Peak EVM in percent (%).

Examples `FETCH:SQUALITY:PEAK:EVM?` might return `4.276`, indicating that the peak EVM is `4.276%`.

FETCH:SQUALITY:PEAK:EVM:DB? (Query Only)

Returns the peak EVM (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:EVM:DB?`

Arguments None

Returns `<NRf>` Peak EVM in dB.

Examples `FETCH:SQUALITY:PEAK:EVM:DB?` might return `-27.358`, indicating that the peak EVM is `-27.358` dB.

FETCh:SQUality:PEAK:EVM:DB:OFFSet? (Query Only)

Returns the peak offset EVM (dB) in the signal quality measurement.

This command is valid when [SENSe]:DDEMod:MODulation:TYPE is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	FETCh:SQUality:PEAK:EVM:DB:OFFSet?
Arguments	None
Returns	<NRf> Peak offset EVM in dB.
Examples	FETCh:SQUality:PEAK:EVM:DB:OFFSet? might return -37.624, indicating the peak offset EVM is -37.624 dB.

FETCh:SQUality:PEAK:EVM:LOCation? (Query Only)

Returns the time at which the EVM is peak.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	FETCh:SQUality:PEAK:EVM:LOCation?
Arguments	None
Returns	<NRf> The time in symbol number at which the EVM is peak. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	FETCh:SQUality:PEAK:EVM:LOCation? might return 68.000, indicating that the EVM is peak at symbol #68.000.

FETCh:SQUality:PEAK:EVM:LOCation:OFFSet? (Query Only)

Returns the time at which the offset EVM is peak.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	FETCh:SQUality:PEAK:EVM:LOCation:OFFSet?
Arguments	None
Returns	<NRf> The time in symbol number at which the offset EVM is peak. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	FETCh:SQUALITY:PEAK:EVM:LOCATION:OFFSET? might return 123.00, indicating that the offset EVM is peak at symbol #123.

FETCh:SQUality:PEAK:EVM:OFFSet? (Query Only)

Returns the peak offset EVM (%) in the signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	FETCh:SQUality:PEAK:EVM:OFFSet?
Arguments	None
Returns	<NRf> Peak offset EVM in percent (%).

Examples `FETCH:SQUALITY:PEAK:EVM:OFFSET?` might return 1.298, indicating the peak offset EVM is 1.298%.

FETCH:SQUALITY:PEAK:FERROR? (Query Only)

Returns the peak FSK error in the signal quality measurement.

This command is valid when `[SENSE]:DDEMod:MODulation:TYPE` is set to FSK2, FSK4, FSK8, or FSK16.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:FERROR?`

Arguments None

Returns <NRF> Peak FSK error in percent (%).

Examples `FETCH:SQUALITY:PEAK:FERROR?` might return 9.136, indicating the peak FSK error is 9.136%.

FETCH:SQUALITY:PEAK:MERROR? (Query Only)

Returns the peak magnitude error (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:MERROR?`

Arguments None

Returns <NRF> Peak magnitude error in percent (%).

Examples `FETCH:SQUALITY:PEAK:MERROR?` might return `3.595`, indicating that the peak magnitude error is 3.595%.

FETCH:SQUALITY:PEAK:MERROR:DB? (Query Only)

Returns the peak magnitude error (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:MERROR:DB?`

Arguments None

Returns `<NRf>` Peak magnitude error in dB.

Examples `FETCH:SQUALITY:PEAK:MERROR:DB?` might return `-28.583`, indicating that the magnitude error is -28.583 dB.

FETCH:SQUALITY:PEAK:MERROR:LOCATION? (Query Only)

Returns the time at which the magnitude error is peak.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:MERROR:LOCATION?`

Arguments None

Returns `<NRf>` The time in symbol number at which the magnitude error is peak. The unit can be changed by the `[SENSE]:DDEMod:TIME:UNITS` command.

Examples `FETCH:SQUALITY:PEAK:MERROR:LOCATION?` might return `68.000`, indicating that the magnitude error is peak at symbol #68.

FETCH:SQUALITY:PEAK:PERROR? (Query Only)

Returns the peak phase error in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:PERROR?`

Arguments None

Returns <NRf> Peak phase error in degrees.

Examples `FETCH:SQUALITY:PEAK:PERROR?` might return `1.907`, indicating that the peak phase error is `1.907 °`.

FETCH:SQUALITY:PEAK:PERROR:LOCATION? (Query Only)

Returns the time at which the phase error is peak.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:PEAK:PERROR:LOCATION?`

Arguments None

Returns <NRf> The time in symbol number at which the phase error is peak.
The unit can be changed by the `[SENSE]:DDEMod:TIME:UNITs` command.

Examples `FETCH:SQUALITY:PEAK:PEERROR:LOCATION?` might return `68.000`, indicating that the phase error is peak at symbol #68.

FETCH:SQUALITY:QUADRATURE:ERROR? (Query Only)

Returns the quadrature error in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:QUADRATURE:ERROR?`

Arguments None

Returns `<NRf>` Quadrature error in degrees.

Examples `FETCH:SQUALITY:QUADRATURE:ERROR?` might return `-14.264E-3`, indicating that the quadrature error is -0.014264° .

FETCH:SQUALITY:RHO? (Query Only)

Returns the ρ (waveform quality) value in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:RHO?`

Arguments None

Returns `<NRf>` ρ value.

Examples `FETCH:SQUALITY:RHO?` might return `998.703E-3`, indicating that ρ is 0.998703.

FETCh:SQUality:RMS:EVM? (Query Only)

Returns the RMS EVM (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax FETCh:SQUality:RMS:EVM?

Arguments None

Returns <NRF> RMS EVM in percent (%).

Examples FETCh:SQUality:RMS:EVM? might return 2.417, indicating that the RMS EVM is 2.417%.

FETCh:SQUality:RMS:EVM:DB? (Query Only)

Returns the RMS EVM (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax FETCh:SQUality:RMS:EVM:DB?

Arguments None

Returns <NRF> RMS EVM in dB.

Examples FETCh:SQUality:RMS:EVM:DB? might return -32.356, indicating that the RMS EVM is -32.356 dB.

FETCh:SQUality:RMS:EVM:DB:OFFSet? (Query Only)

Returns the RMS offset EVM (dB) in the signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	FETCh:SQUality:RMS:EVM:DB:OFFSet?
Arguments	None
Returns	<NRf> RMS offset EVM in dB.
Examples	FETCh:SQUality:RMS:EVM:DB:OFFSet? might return -41.276, indicating the RMS offset EVM is -41.276 dB.

FETCh:SQUality:RMS:EVM:OFFSet? (Query Only)

Returns the RMS offset EVM (%) in the signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Fetch commands
Syntax	FETCh:SQUality:RMS:EVM:OFFSet?
Arguments	None
Returns	<NRf> RMS offset EVM in percent (%).

Examples `FETCH:SQUALITY:RMS:EVM:OFFSET?` might return 0.783, indicating the RMS offset EVM is 0.783%.

FETCH:SQUALITY:RMS:FERROR? (Query Only)

Returns the RMS FSK error percent in the signal quality measurement.

This command is valid when `[SENSE]:DDEMod:MODulation:TYPE` is set to FSK2, FSK4, FSK8, or FSK16.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:RMS:FERROR?`

Arguments None

Returns <NRF> RMS FSK error in percent (%).

Examples `FETCH:SQUALITY:RMS:FERROR?` might return 1.815, indicating the RMS FSK error is 1.815%.

FETCH:SQUALITY:RMS:MER:DB? (Query Only)

Returns the RMS MER (Modulation Error Ratio) in dB in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:RMS:MER:DB?`

Arguments None

Returns <NRF> RMS MER in dB.

Examples `FETCH:SQUALITY:RMS:MERRor:DB?` might return `27.394`, indicating that the RMS MER is 27.394 dB.

FETCH:SQUALITY:RMS:MERRor? (Query Only)

Returns the RMS magnitude error (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:RMS:MERRor?`

Arguments None

Returns `<NRf>` RMS magnitude error in percent (%).

Examples `FETCH:SQUALITY:RMS:MERRor?` might return `1.837`, indicating that the RMS magnitude error is 1.837%.

FETCH:SQUALITY:RMS:MERRor:DB? (Query Only)

Returns the RMS magnitude error (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax `FETCH:SQUALITY:RMS:MERRor:DB?`

Arguments None

Returns `<NRf>` RMS MERRor in dB.

Examples `FETCH:SQUALITY:RMS:MERRor:DB?` might return `-34.706`, indicating that the magnitude error is -34.706 dB.

FETCh:SQUality:RMS:PERRor? (Query Only)

Returns the RMS phase error in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Fetch commands

Syntax FETCh:SQUality:RMS:PERRor?

Arguments None

Returns <NRf> RMS phase error in degrees.

Examples FETCh:SQUality:RMS:PERRor? might return 893.472E-3, indicating that the RMS phase error is 0.893472 °.

FETCh:SQUality:SYMBol:LENGth? (Query Only)

Returns the number of analyzed symbols.

Group Fetch commands

Syntax FETCh:SQUality:SYMBol:LENGth?

Related Commands

Returns <NR1> indicates the length of the synch word in symbols.

Examples FETCh:SQUality:SYMBol:LENGth? might return 3, indicating the length is three symbols.

FETCh:SQUality:SYMBol:RATE? (Query Only)

Returns the value of the calculated symbol rate in Hz.

Conditions Measurement views: Signal quality

It is valid when the modulation type is 2|4|8|16FSK and [:SENSE]:DDEMod:SYMBOL:RATE:SEARCH is ON.

Group Fetch commands

Syntax FETCH:SQUALITY:SYMBOL:RATE?

Related Commands [\[SENSE\]:DDEMod:SYMBOL:RATE:SEARCH](#)

Returns <NRF> is the calculated symbol rate in Hz.

Examples FETCH:SQUALITY:SYMBOL:RATE? might return 95.24E+3, indicating the calculated symbol rate is 95.24 kHz.

FETCH:SQUALITY:SYMBOL:RATE:ERROR? (Query Only)

Returns the value of the symbol rate error in percent (%).

Conditions Measurement views: Signal quality

It is valid when the modulation type is 2|4|8|16FSK and [:SENSE]:DDEMod:SYMBOL:RATE:SEARCH is ON.

Group Fetch commands

Syntax FETCH:SQUALITY:SYMBOL:RATE:ERROR?

Related Commands [\[SENSE\]:DDEMod:SYMBOL:RATE:SEARCH](#)

Returns <NRF> is the symbol error percent (%).

Examples FETCH:SQUALITY:SYMBOL:RATE:ERROR? might return -0.002, indicating that the symbol rate error is -0.002%.

FETCH:TDLIAGRAM:FERROR? (Query Only)

Returns the frequency error in the trellis diagram measurement.

Conditions	Measurement views: Trellis diagram
Group	Fetch commands
Syntax	FETCh:TDIagram:FERRor?
Arguments	None
Returns	<freq_error> ::= <Nrf> is the frequency error in Hz.
Examples	FETCh:TDIAGRAM:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

FETCh:TDIagram:TRACe? (Query Only)

Returns the Trellis diagram trace data.

Conditions	Measurement views: Trellis diagram
Group	Fetch commands
Syntax	FETCh:TDIagram:TRACe?
Arguments	None
Returns	<p>#<num_digit><num_byte><Y(1)><X(1)><Y(2)><X(2)>...<Y(n)><X(n)></p> <p>Where</p> <ul style="list-style-type: none"> <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <Y(n)><X(n)> is the phase in degrees and the time in symbols pair at the nth data point. The 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	FETCh:TDIAGRAM:TRACE? might return #3160xxxx... (160-byte data) for the Trellis diagram trace.

FETCH:TOVerview? (Query Only)

Returns the trace data in the time overview.

Conditions	Measurement views: Time overview
Group	Fetch commands
Syntax	FETCH:TOVerview?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude in dBm at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	FETCH:TOVERVIEW? might return #43204xxxx... (3204-byte data) for the trace in the time overview.

*IDN? (Query Only)

Returns the analyzer identification code.

Conditions	Measurement views: All
Group	IEEE common commands
Syntax	*IDN?
Arguments	None
Returns	The analyzer identification code in the following format TEKTRONIX, RSA61XXA, <serial_number>, <firmware_version>

Where
 TEKTRONIX indicates that the manufacturer is Tektronix.
 RSA61XXA is the model number (RSA6106A or RSA6114A).
 <serial_number> is the serial number.
 <firmware_version> is the firmware version.

Examples *IDN? might return the response
 TEKTRONIX, RSA6114A, B000111, FV1.0.1500.

INITiate:CONTInuous

Determines whether to place the analyzer in the single or the continuous acquisition mode.

Conditions Measurement views: All

Group Initiate commands

Syntax INITiate:CONTInuous { OFF | ON | 0 | 1 }
 INITiate:CONTInuous?

Related Commands [INITiate\[:IMMediate\]](#)

Arguments OFF or 0 places the analyzer in the single acquisition mode. To initiate the acquisition, use the INITiate[:IMMediate] command. To stop acquisition when a trigger is not present, and to avoid a 2.7 hour time-out, send the free-run trigger command, TRIGger:SEQuence:STATus 0. Then, send the command INITiate:CONTInuous OFF. This sequence ensures a minimal delay before the INIT:CONT OFF command completes.

ON or 1 places the analyzer in the continuous acquisition mode. To initiate the acquisition, use the INITiate[:IMMediate] command. To stop the acquisition in the continuous mode, send the following command: INITiate:CONTInuous OFF

Examples INITIATE:CONTINUOUS ON places the analyzer in the continuous acquisition mode.

INITiate[:IMMediate] (No Query Form)

Starts input signal acquisition.

NOTE. *It is an overlapped command, which does not finish executing before the next command starts executing. Use the *OPC(?) and *WAI commands to synchronize all pending operations to the execution of this command.*

Conditions	Measurement views: All
Group	Initiate commands
Syntax	INITiate[:IMMEDIATE]
Related Commands	*OPC, *TRG, *WAI, INITiate:CONTinuous
Arguments	None
Examples	INITIATE:IMMEDIATE starts input signal acquisition.

INPut:CORRection:EXTernal:EDIT<x>:INTerpolation

Sets or queries the interpolation setting to use with the indicated external gain table.

Conditions	Measurement views: All
Group	Input commands
Syntax	INPut:CORRection:EXTernal:EDIT<x>:INTerpolation { LINear LOGarithmic } INPut:CORRection:EXTernal:EDIT<x>:INTerpolation
Related Commands	INPut:CORRection:EXTernal:EDIT<x>:NEW
Arguments	LINear select when the frequency scale of the spectrum or spurious measurements are linear. LOGarithmic select when the frequency scale of the spectrum is logarithmic.

Examples `INPut:CORRection:EXTErnal:EDIT1:INTERpolation LINEar` uses linear interpolation when applying External correction Table one (1) to the chosen waveforms.

INPut:CORRection:EXTErnal:EDIT<x>:NEW

Creates the indicated (x) external loss table from a series of frequency and gain value pairs.

Conditions Measurement views: All

Group Input commands

Syntax `INPut:CORRection:EXTErnal:EDIT<x>:NEW
<freq(1)>, <gain(1)>, <freq(2)>, <gain(2)>, ..., <freq(n)>, <gain(n)>
INPut:CORRection:EXTErnal:EDIT<x>:NEW?`

Related Commands [INPut:CORRection:EXTErnal:TYPE](#)

Arguments `<freq(n)>, <gain(n)>` specifies a pair of frequency (<NR3> in Hz) and gain (+ | -<NR3> in dB) in the external correction table.

The setting range is:

Frequency: 0 to 6.2 GHz for the RSA6106A) and 0 to 14 GHz for the RSA6114A.

Loss: -50 to +30 dB. Negative values indicate loss and positive values indicate gain. Resolution is 0.1 dB.

Examples `INPut:CORRection:EXTErnal:EDIT?:NEW 1.0E+9, -2.2,
-1.5E+9, -2.3` creates the External correction Table specifying a loss of 2.2 dB at 1 GHz and a loss of 2.3 dB at 1.5 GHz.

INPut:CORRection:EXTErnal:TYPE

Sets or queries the data type to use when applying the external loss table corrections.

Conditions Measurement views: All

Group Input commands

Syntax `INPut:CORRection:EXTErnal:TYPE { TRACe | DATA }`
`INPut:CORRection:EXTErnal:TYPE`

Related Commands [INPut:CORRection:EXTErnal:EDIT<x>:NEW](#)

Arguments TRACe selects traces in the Spectrum, Spectrogram, Spurious, and Amplitude versus Time views. Selecting TRACe disables the CALibration:CORRection:EXTErnal:GAIN:STATe command.

DATA selects all acquired data. Selecting DATA enables the CALibration:CORRection:EXTErnal:GAIN:STATe command.

Examples `INPut:CORRection:EXTErnal:TYPE TRACe` selects traces to apply the external loss table corrections.

INPut:{MLEVe|RLEVe}

Sets or queries the reference level.

Conditions Measurement views: All

Group Input commands

Syntax `INPut:{MLEVe|RLEVe} <value>`
`INPut:{MLEVe|RLEVe}?`

Arguments `<value> ::= <NRF>` specifies the reference level. Range: -170 to +50 dBm.

Examples `INPut:RLEVEL -10` sets the reference level to -10 dBm.

INPut[:RF]:ATTenuation

Sets or queries the input attenuation. Programming a specified attenuation sets INPut[:RF]:ATTenuation:AUTO OFF.

Conditions Measurement views: All

Group Input commands

Syntax `INPut[:RF]:ATTenuation <value>`
`INPut[:RF]:ATTenuation?`

Related Commands [INPut\[:RF\]:ATTenuation:AUTO](#)

Arguments `<value>::=<NR1>` specifies the input attenuation.
Range: 0 to 75 dB in 5 dB steps.

Examples `INPUT:RF:ATTENUATION 20` sets the input attenuation to 20 dB.

INPut[:RF]:ATTenuation:AUTO

Determines whether to set the input attenuation automatically or manually.

Conditions Measurement views: All

Group Input commands

Syntax `INPut[:RF]:ATTenuation:AUTO { OFF | ON | 0 | 1 }`
`INPut[:RF]:ATTenuation:AUTO?`

Arguments `OFF` or `0` specifies that the input attenuation is set manually.
To set it, use the [INPut\[:RF\]:ATTenuation](#) command.

`ON` or `1` specifies that the input attenuation is set automatically according to the reference level.

Examples `INPUT:RF:ATTENUATION:AUTO ON` specifies that the input attenuation is set automatically.

INPut[:RF]:ATTenuation:MONitor:STATe

Determines whether to enable or disable to monitor attenuator use.

Conditions Measurement views: All

Group Input commands

Syntax	<code>INPut[:RF]:ATTenuation:MONitor:STATE { OFF ON 0 1 }</code> <code>INPut[:RF]:ATTenuation:MONitor:STATE?</code>
Arguments	OFF or 0 disables to monitor attenuator use. ON or 1 enables to monitor attenuator use.
Examples	<code>INPUT:RF:ATTENUATION:MONITOR:STATE ON</code> enables to monitor attenuator use.

INPut[:RF]:GAIN:STATE

Determines whether to enable or disable the internal pre-amp.

Conditions	Measurement views: All (Option 01 only)
Group	Input commands
Syntax	<code>INPut[:RF]:GAIN:STATE { OFF ON 0 1 }</code> <code>INPut[:RF]:GAIN:STATE?</code>
Arguments	OFF or 0 disables the internal pre-amp. ON or 1 enables the internal pre-amp.
Examples	<code>INPUT:RF:GAIN:STATE ON</code> enables the internal pre-amp.

MMEMory:{AM|FM|PM}:LOAD:TRACe (No Query Form)

Loads the AM/FM/PM measurement trace data from the specified file.

Conditions	Measurement views: AM, FM, PM
Group	Mass memory commands
Syntax	<code>MMEMory:{AM FM PM}:LOAD:TRACe <file_name></code>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .AmVsTime (AM), .FmVsTime (FM), or .PmVsTime (PM). You can omit the extension.

Examples MMEMORY:AM:LOAD:TRACE "Sample1" loads the trace data from the *Sample1.AmVsTime* file in the AM measurement.

MMEMory:{AM|FM|PM}:SHOW:TRACe<x>

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: AM, FM, PM

Group Mass memory commands

Syntax MMEMORY:{AM|FM|PM}:SHOW:TRACe<x> { OFF | ON | 0 | 1 }
MMEMory:{AM|FM|PM}:SHOW:TRACe<x>?

Related Commands [MMEMory:{AM|FM|PM}:LOAD:TRACe](#)

Arguments OFF or 0 disables display of the recalled trace.
ON or 1 enables display of the recalled trace.

Examples MMEMORY:FM:SHOW:TRACe2 ON enables display of the recalled data loaded in Trace2.

MMEMory:{AM|FM|PM}:STORE:TRACe (No Query Form)

Stores the AM/FM/PM measurement trace data in the specified file.

Conditions Measurement views: AM, FM, PM

Group Mass memory commands

Syntax MMEMORY:{AM|FM|PM}:STORE:TRACe <file_name>

Arguments `<file_name>::=<string>` specifies the file from which to load trace data. The file extension is `.AmVsTime` (AM), `.FmVsTime` (FM), or `.PmVsTime` (PM). You can omit the extension.

Examples `MMEMORY:AM:STORE:TRACE "Sample1"` stores the trace data in the `Sample1.AmVsTime` file in the AM measurement.

MMEMory:AVTime:LOAD:TRACe<x> (No Query Form)

Loads the Amplitude versus Time trace data from the specified file.

The parameter `<x>` = 1 to 3; Trace 4 (math trace) is invalid.

Conditions Measurement views: Amplitude versus Time

Group Mass memory commands

Syntax `MMEMory:AVTime:LOAD:TRACe<x> <file_name>`

Arguments `<file_name>::=<string>` specifies the file from which to load trace data. The file extension is `.AmplVsTime`. You can omit the extension.

Examples `MMEMORY:AVTIME:LOAD:TRACE1 "Sample1"` loads Trace 1 data from the `Sample1.AmplVsTime` file.

MMEMory:AVTime:SHOW:TRACe<x>

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: Amplitude versus Time

Group Mass memory commands

Syntax `MMEMory:AVTime:SHOW:TRACe<x> { OFF | ON | 0 | 1 }`
`MMEMory:AVTime:SHOW:TRACe<x>?`

Related Commands	MMEMory:AVTime:LOAD:TRACe<x>
Arguments	OFF or 0 disables display of the recalled trace. ON or 1 enables display of the recalled trace.
Examples	MMEMory:AVTime:SHOW:TRACe2 ON enables display of the recalled data loaded in Trace2.

MMEMory:AVTime:STORE:TRACe<x> (No Query Form)

Stores the Amplitude versus Time trace data in the specified file.

The parameter <x> = 1 to 4; All traces are valid.

Conditions	Measurement views: Amplitude versus Time
Group	Mass memory commands
Syntax	MMEMory:AVTime:STORE:TRACe<x> <file_name>
Arguments	<file_name>::=<string> specifies the file in which to store trace data. The file extension is .AmplVsTime. You can omit the extension.
Examples	MMEMORY:AVTIME:STORE:TRACE1 "Sample1" stores Trace 1 data in the <i>Sample1.AmplVsTime</i> file.

MMEMory:CALibration:LOAD:CORRection:EXTErnal:EDIT<x> (No Query Form)

Loads the external loss table from a specified file.

The parameter <x> = 1 to 3 represent External Loss Table 1 to 3, respectively.

Conditions	Measurement views: All
Group	Mass memory commands
Syntax	MMEMory:CALibration:LOAD:CORRection:EXTErnal:EDIT<x> <file_name>

Arguments `<file_name>::=<string>` specifies the file to load the external loss table from. The file extension is .csv. You can omit the extension.

Examples `MMEMORY:CALIBRATION:LOAD:CORRECTION:EXTERNAL:EDIT1 "Table1"` loads the External Loss Table 1 from the *Table1.csv* file.

MMEMory:CALibration:STORE:CORRection:EXTErnal:EDIT<x> (No Query Form)

Stores the external loss table to a specified file.

The parameter `<x>` = 1 to 3 represent External Loss Table 1 to 3, respectively.

Conditions Measurement views: All

Group Mass memory commands

Syntax `MMEMory:CALibration:STORE:CORRection:EXTErnal:EDIT<x>
<file_name>`

Arguments `<file_name>::=<string>` specifies the file to store the external loss table to. The file extension is .csv. You can omit the extension.

Examples `MMEMORY:CALIBRATION:STORE:CORRECTION:EXTERNAL:EDIT1 "Table1"` stores the External Loss Table 1 to the *Table1.csv* file.

MMEMory:CCDF:LOAD:TRACe<x> (No Query Form)

Loads the CCDF trace data from the specified file.

Conditions Measurement views: CCDF

Group Mass memory commands

Syntax `MMEMory:CCDF:LOAD:TRACe<x> <file_name>`

Arguments `<file_name>::=<string>` specifies the file from which to load trace data. The file extension is .CCDF. You can omit the extension.

Examples `MMEMORY:CCDF:LOAD:TRACE1 "Sample1"` loads Trace 1 data from the *Sample1.CCDF* file.

MMEMory:CCDF:SHOW:TRACe<x>

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: CCDF

Group Mass memory commands

Syntax `MMEMory:CCDF:SHOW:TRACe<x> { OFF | ON | 0 | 1 }`
`MMEMory:CCDF:SHOW:TRACe<x>?`

Related Commands [MMEMory:CCDF:LOAD:TRACe<x>](#)

Arguments OFF or 0 disables display of the recalled trace.
 ON or 1 enables display of the recalled trace.

Examples `MMEMory:CCDF:SHOW:TRACe2 ON` enables display of the recalled data loaded in Trace2.

MMEMory:CCDF:STORE:TRACe<x> (No Query Form)

Stores the CCDF trace data in the specified file.

Conditions Measurement views: CCDF

Group Mass memory commands

Syntax `MMEMory:CCDF:STORE:TRACe<x> <file_name>`

Arguments `<file_name>::=<string>` specifies the file in which to store trace data. The file extension is `.CCDF`. You can omit the extension.

Examples `MMEMORY:CCDF:STORE:TRACE1 "Sample1"` stores Trace 1 data in the *Sample1.CCDF* file.

MMEMory:DDEMod:LOAD:FILTer:MEASurement:UOTHer (No Query Form)

Loads a user-defined measurement filter from the specified file.

Group Mass memory commands

Syntax `MMEMory:DDEMod:LOAD:FILTer:MEASurement:UOTHer <file_name>`

Related Commands [\[SENSe\]:DDEMod:FILTer:REFerence](#)
[\[SENSe\]:DDEMod:FILTer:MEASurement](#)

Arguments `<file_name>::=<string>` specifies the filter file to load.

Examples `MMEMory:DDEMod:LOAD:FILTer:MEASurement:UOTHer "Table2"` loads User other filter from the file *Table2.csv*.

MMEMory:DDEMod:LOAD:FILTer:MEASurement:USER<x> (No Query Form)

Loads the user-defined measurement filter from the specified file. The parameter `<x>` specifies one of the User Meas Filters, 1 to 3. The filter file must have a `.csv` file extension, though you may omit the file extension in the command line.

Group Mass memory commands

Syntax `MMEMory:DDEMod:LOAD:FILTer:MEASurement:USER<x> <file_name>`

Related Commands [\[SENSe\]:DDEMod:FILTer:REFerence](#)
[\[SENSe\]:DDEMod:FILTer:MEASurement](#)

Arguments `<file_name>::=<string>` specifies the filter file to load.

Examples `MMEMory:DDEMod:LOAD:FILTer:MEASurement:USER1 "Table1"` loads User Meas Filter 1 from the file *Table1.csv*.

MMEMory:DDEMod:LOAD:FILTer:REFerence:UOTHer (No Query Form)

Loads the specified user-defined reference filter, UOTHer, from a specified file.

Group Mass memory commands

Syntax MMEMory:DDEMod:LOAD:FILTer:REFerence:UOTHer <file_name>

Related Commands [\[SENSe\]:DDEMod:FILTer:REFerence](#)
[\[SENSe\]:DDEMod:FILTer:MEASurement](#)

Arguments <file_name>::=<string>specifies the reference filter file to load. The file extension is type .csv.

Examples MMEMory:DDEMOD:LOAD:FILTer:REFerence:UOTHer "FinalFilt" loads the filter file FinalFilt.csv into the filter reference UOTHer.

MMEMory:DDEMod:LOAD:FILTer:REFerence:USER<x> (No Query Form)

Loads the specified user-defined reference filter, USER1 | 2 | 3 from a specified file.

Group Mass memory commands

Syntax MMEMory:DDEMod:LOAD:FILTer:REFerence:USER<x> <file_name>

Related Commands [\[SENSe\]:DDEMod:FILTer:REFerence](#)

Arguments <file_name>::=<string>specifies the reference filter file to load. The file extension is type .csv.

Examples MMEMory:DDEMOD:LOAD:FILTer:REFerence:USER2 "DUTFilt2" loads the filter file DUTfilt2.csv into the filter reference USER2.

MMEMory:DDEMod:LOAD:SYMBOL:MAP (No Query Form)

Loads the specified symbol map filename. The setting correlates to the field, User Symbol Map (per Modulation Type) on the Advanced Params tab in the Digital Modulation settings.

Group Mass memory commands

Syntax MMEMory:DDEMod:LOAD:SYMBOL:MAP <file_name>

Related Commands [\[SENSe\]:DDEMod:MODulation:TYPE](#)

Arguments <file_name>::=<string> specifies the symbol map file to load. The file extension is type .txt.

Examples MMEMory:DDEMod:LOAD:SYMBOL:MAP "C:\usymmap.txt" identifies the file to load for the symbol map.

MMEMory:DPSA:LOAD:TRACe<x> (No Query Form)

Loads the DPX spectrum trace data from the specified file.

The parameter <x> = 1, 2, 3, or 5; TRACe4 (math trace) is invalid.

Conditions Measurement views: DPX spectrum

Group Mass memory commands

Syntax MMEMory:DPSA:LOAD:TRACe<x> <file_name>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .dpt. You can omit the extension.

Examples MMEMORY:DPSA:LOAD:TRACE1 "Sample1" loads Trace 1 data from the *Sample1.dpt* file.

MMEMory:DPSA:SHOW:TRACe<x>

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views:DPX spectrum

Group Mass memory commands

Syntax MMEMory:DPSA:SHOW:TRACe<x> { OFF | ON | 0 | 1 }
MMEMory:DPSA:SHOW:TRACe<x>?

Related Commands [MMEMory:DPSA:LOAD:TRACe<x>](#)

Arguments OFF or 0 disables display of the recalled trace.
ON or 1 enables display of the recalled trace.

Examples MMEMory:DPSA:SHOW:TRACe2 ON enables display of the recalled data loaded in Trace2.

MMEMory:DPSA:STORE:TRACe<x> (No Query Form)

Stores the DPX spectrum trace data in the specified file.

The parameter <x> = 1 to 5; All traces are valid.

Conditions Measurement views: DPX spectrum

Group Mass memory commands

Syntax MMEMory:DPSA:STORE:TRACe<x> <file_name>

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .dpt. You can omit the extension.

Examples MMEMORY:DPSA:STORE:TRACE1 "Sample1" stores Trace 1 data in the *Sample1.dpt* file.

MMEMory:FVTime:LOAD:TRACe (No Query Form)

Loads the Frequency versus Time trace data from the specified file.

Conditions Measurement views: Frequency versus Time

Group Mass memory commands

Syntax MMEMory:FVTime:LOAD:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .FreqVsTime. You can omit the extension.

Examples MMEMory:FVTime:LOAD:TRACe "Sample1" loads the Frequency versus Time trace data from the *Sample1.FreqVsTime* file.

MMEMory:FVTime:SHOW:TRACe<x>

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: Frequency versus Time

Group Mass memory commands

Syntax MMEMory:FVTime:SHOW:TRACe<x> { OFF | ON | 0 | 1 }
MMEMory:FVTime:SHOW:TRACe<x>?

Related Commands [MMEMory:FVTime:LOAD:TRACe](#)

Arguments OFF or 0 disables display of the recalled trace.
ON or 1 enables display of the recalled trace.

Examples MMEMory:FVTime:SHOW:TRACe2 ON enables display of the recalled data loaded in Trace2.

MMEMemory:FVTime:STORE:TRACe (No Query Form)

Stores the Frequency versus Time trace data in the specified file.

Conditions	Measurement views: Frequency versus Time
Group	Mass memory commands
Syntax	MMEMemory:FVTime:STORE:TRACe <file_name>
Arguments	<file_name>::=<string> specifies the file in which to store trace data. The file extension is .FreqVsTime. You can omit the extension.
Examples	MMEMEMORY:FVTIME:STORE:TRACE "Sample1" stores the Frequency versus Time trace data in the <i>Sample1.FreqVsTime</i> file.

MMEMemory:IQVTime:LOAD:TRACe:I (No Query Form)

Loads I trace data from the specified file.

Conditions	Measurement views: RF I&Q versus Time
Group	Mass memory commands
Syntax	MMEMemory:IQVTime:LOAD:TRACe:I <file_name>
Arguments	<file_name>::=<string> specifies the file from which to load trace data. The file extension is .RFIQVsTime. You can omit the extension.
Examples	MMEMEMORY:IQVTIME:LOAD:TRACE:I "Sample1" loads the I trace data from the <i>Sample1.RFIQVsTime</i> file.

MMEMemory:IQVTime:LOAD:TRACe:Q (No Query Form)

Loads Q trace data from the specified file.

Conditions	Measurement views: RF I&Q versus Time
-------------------	---------------------------------------

Group	Mass memory commands
Syntax	<code>MMEMory:IQVTime:LOAD:TRACe:Q <file_name></code>
Arguments	<code><file_name>::=<string></code> specifies the file from which to load trace data. The file extension is <code>.RFIQVsTime</code> . You can omit the extension.
Examples	<code>MMEMORY:IQVTIME:LOAD:TRACE:Q "Sample2"</code> loads the I trace data from the <code>Sample2.RFIQVsTime</code> file.

MMEMory:IQVTIME:SHOW:TRACe:I

Enables display of a recalled trace file in Trace. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions	Measurement views: RF I&Q versus Time
Group	Mass memory commands
Syntax	<code>MMEMory:IQVTIME:SHOW:TRACe:I { OFF ON 0 1 }</code> <code>MMEMory:IQVTIME:SHOW:TRACe:I?</code>
Related Commands	MMEMory:IQVTime:LOAD:TRACe:I
Arguments	OFF or 0 disables display of the recalled trace. ON or 1 enables display of the recalled trace.
Examples	<code>MMEMory:IQVTIME:SHOW:TRACe:I ON</code> enables display of the recalled data loaded in the Trace.

MMEMory:IQVTIME:SHOW:TRACe<x>:Q

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions	Measurement views: RF I&Q versus Time
Group	Mass memory commands
Syntax	MMEMory:IQVTIME:SHOW:TRACe<x>:Q { OFF ON 0 1 } MMEMory:IQVTIME:SHOW:TRACe<x>:Q?
Related Commands	MMEMory:IQVTIME:SHOW:TRACe<x>:Q
Arguments	OFF or 0 disables display of the recalled trace. ON or 1 enables display of the recalled trace.
Examples	MMEMory:IQVTIME:SHOW:TRACe3:Q ON enables display of the recalled data loaded in Trace3.

MMEMory:IQVTime:STORE:TRACe:I (No Query Form)

Stores I trace data in the specified file.

Conditions	Measurement views: RF I&Q versus Time
Group	Mass memory commands
Syntax	MMEMory:IQVTime:STORE:TRACe:I <file_name>
Arguments	<file_name>::=<string> specifies the file in which to store trace data. The file extension is .RFIQVsTime. You can omit the extension.
Examples	MMEMORY:IQVTIME:STORE:TRACe:I "Sample1" stores the I trace data in the <i>Sample1.RFIQVsTime</i> file.

MMEMory:IQVTime:STORE:TRACe:Q (No Query Form)

Stores Q trace data in the specified file.

Conditions	Measurement views: RF I&Q versus Time
-------------------	---------------------------------------

Group	Mass memory commands
Syntax	<code>MMEMemory:IQVTime:STORe:TRACe:Q <file_name></code>
Arguments	<code><file_name>::=<string></code> specifies the file in which to store trace data. The file extension is <code>.RFIQVsTime</code> . You can omit the extension.
Examples	<code>MMEMemory:IQVTime:STORe:TRACe:Q "Sample2"</code> stores the Q trace data in the <code>Sample2.RFIQVsTime</code> file.

MMEMemory:LOAD:IQ (No Query Form)

Loads time-domain IQ waveform into the acquisition memory from a file.

Conditions	Measurement views: All
Group	Mass memory commands
Syntax	<code>MMEMemory:LOAD:IQ <file_name></code>
Arguments	<code><file_name>::=<string></code> specifies the file to load IQ data from. The file extension is <code>.tiq</code> . You can omit the extension.
Examples	<code>MMEMemory:LOAD:IQ "IQ1"</code> loads IQ data from the <code>IQ1.tiq</code> file.

MMEMemory:LOAD:STATE (No Query Form)

Loads the instrument setup from a specified file for the currently selected view.

Conditions	Measurement views: All
Group	Mass memory commands
Syntax	<code>MMEMemory:LOAD:STATE <file_name></code>

Arguments <file_name>::=<string> specifies the file to load the instrument setup from. The file extension is .setup. You can omit the extension.

Examples `MMEMORY:LOAD:STATE "STATE1"` loads the instrument setup from the *STATE1.setup* file.

MMEMory:LOAD:TRACe (No Query Form)

Loads the trace data from a specified file for the currently selected view.

Conditions Measurement views (See Table 2-34.)

Group Mass memory commands

Syntax `MMEMory:LOAD:TRACe <file_name>`

Related Commands [MMEMory:STORe:TRACe](#)

Arguments <file_name>::=<string> specifies the file to load the trace data from. The file extension is named for the measurement view as shown in the following table. The trace file is not available in some views which are indicated by "NA" in the file extension column.

For the views that allow multiple-trace display, select the trace to load or store using the command listed in the trace selection column in the following table. You can load the specified trace with any trace data that you saved in the view if the traces have the same units. For example, you can load Trace 2 with Trace 1 data that you saved.

Table 2-34: Trace file extension and trace selection command

Display group	Measurement view	File extension	Trace selection
General signal viewing	Spectrum	Specan	TRACe<x>:SPECtrum:SElect
	DPX spectrum	dpt	TRACe<x>:DPSA:SElect
	Amplitude versus Time	AmplVsTime	TRACe<x>:AVTime:SElect
	Frequency versus Time	FreqVsTime	NA
	Phase versus Time	PhaseVsTime	NA
	RF I&Q versus Time	RFIQVsTime	NA
	Spectrogram	Sogram	NA
	Time overview	NA	NA

Table 2-34: Trace file extension and trace selection command (cont.)

Display group	Measurement view	File extension	Trace selection
General purpose analog modulation (Option 21 only)	AM	AmVsTime	NA
	FM	FmVsTime	NA
	PM	PmVsTime	NA
General purpose digital modulation (Option 21 only)	Constellation	NA	NA
	Demodulated I & Q versus Time	NA	NA
	Eye Diagram	NA	NA
	EVM versus Time	NA	NA
	Frequency Deviation versus Time	NA	NA
	Magnitude error versus Time	NA	NA
	Phase error versus Time	NA	NA
	Signal quality	NA	NA
	Symbol table	NA	NA
	Trellis Diagram	NA	NA
RF measurements	CCDF	CCDF	TRACe<x>:CCDF:SElect
	Channel power and ACPR	NA	NA
	MCPR	NA	NA
	Occupied Bandwidth	NA	NA
	Phase noise (Option 11 only)	PhaseNoise	TRACe<x>:PNOise:SElect
	Spurious	NA	NA
Pulsed RF (Option 20 only)	Pulse statistics	NA	NA
	Pulse table	NA	NA
	Pulse trace	NA	NA

Examples `MMEMORY:LOAD:TRACE "TRACE1"` loads the trace data from the *TRACE1.Specan* file when the spectrum view is selected.

MMEMory:PHVTime:LOAD:TRACe (No Query Form)

Loads the Phase versus Time trace data from the specified file.

Conditions Measurement views: Phase versus Time

Group Mass memory commands

Syntax `MMEMory:PHVTime:LOAD:TRACe <file_name>`

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .PhaseVsTime. You can omit the extension.

Examples `MMEMORY:PHVTIME:LOAD:TRACE "Sample1"` loads the Phase versus Time trace data from the *Sample1.PhaseVsTime* file.

MMEMory:PHVTime:SHOW:TRACe

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: Phase versus Time

Group Mass memory commands

Syntax `MMEMory:PHVTime:SHOW:TRACe { OFF | ON | 0 | 1 }`
`MMEMory:PHVTime:SHOW:TRACe?`

Related Commands [MMEMory:PHVTime:LOAD:TRACe](#)

Arguments OFF or 0 disables display of the recalled trace.
 ON or 1 enables display of the recalled trace.

Examples `MMEMory:PHVTIME:SHOW:TRACe ON` enables display of the recalled data loaded in theTrace.

MMEMory:PHVTime:STORE:TRACe (No Query Form)

Stores the Phase versus Time trace data in the specified file.

Conditions Measurement views: Phase versus Time

Group Mass memory commands

Syntax `MMEMory:PHVTime:STORE:TRACe <file_name>`

Arguments `<file_name>::=<string>` specifies the file in which to store trace data. The file extension is `.PhaseVsTime`. You can omit the extension.

Examples `MMEMORY:PHVTIME:STORE:TRACE "Sample1"` stores the Phase versus Time trace data in the `Sample1.PhaseVsTime` file.

MMEMory:PNOise:LOAD:TRACe<x> (No Query Form)

Loads the Phase Noise trace data from the specified file. The parameter `<x> = 1` or `2`; only Trace1 and Trace2 are used for Phase Noise measurement.

Conditions Measurement views: Phase noise

Group Mass memory commands

Syntax `MMEMory:PNOise:LOAD:TRACe<x> <file_name>`

Arguments `<file_name>::=<string>` specifies the file from which to load trace data.

Examples `MMEMORY:PNOISE:LOAD:TRACE1 "wfm1"` loads Trace1 data from the `Wfm1` file.

MMEMory:PNOise:SHOW:TRACe<x>

Enables display of a recalled Phase Noise trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: Phase noise

Group Mass memory commands

Syntax `MMEMory:PNOise:SHOW:TRACe<x> { OFF | ON | 0 | 1 }`
`MMEMory:PNOise:SHOW:TRACe<x>?`

Related Commands [MMEMory:PNOise:LOAD:TRACe<x>](#)

- Arguments** OFF or 0 disables display of the recalled trace.
ON or 1 enables display of the recalled trace.
- Examples** `MMEMemory:PNOise:SHOW:TRACe1 ON` enables display of the recalled data loaded in Trace1.

MMEMemory:PNOise:STORE:TRACe<x> (No Query Form)

Stores the Phase Noise trace data in the specified file. The parameter <x> = 1 or 2; only Trace1 and Trace2 are used for Phase Noise measurement.

- Conditions** Measurement views: Phase noise
- Group** Mass memory commands
- Syntax** `MMEMemory:PNOise:STORE:TRACe<x> <file_name>`
- Arguments** `<file_name>::=<string>` specifies the file in which to store trace data.
- Examples** `MMEMemory:PNOISE:STORE:TRACe1 "WFM1"` stores Trace 1 data in the WFM1 file.

MMEMemory:SGRam:LOAD:TRACe (No Query Form)

Loads the Spectrogram trace data from the specified file. No trace number is needed or allowed.

- Conditions** Measurement views: Spectrogram
- Group** Mass memory commands
- Syntax** `MMEMemory:SGRam:LOAD:TRACe <file_name>`
- Arguments** `<file_name>::=<string>` specifies the file from which to load trace data. The file extension is .sogram. You can omit the extension.

Examples `MMEMORY:SGRAM:LOAD:TRACE5 "Spec2"` loads Trace5 data from the file *Spec2.sogram*.

MMEMory:SGRam:SHOW:TRACe

Enables display of a recalled trace file in Trace. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: Spectrogram

Group Mass memory commands

Syntax `MMEMory:SGRam:SHOW:TRACe { OFF | ON | 0 | 1 }`
`MMEMory:SGRam:SHOW:TRACe?`

Related Commands [MMEMory:SGRam:LOAD:TRACe](#)

Arguments OFF or 0 disables display of the recalled trace.
ON or 1 enables display of the recalled trace.

Examples `MMEMory:SGRAM:SHOW:TRACe ON` enables display of the recalled data loaded in Trace.

MMEMory:SGRam:STORe:TRACe (No Query Form)

Stores the Spectrogram trace data in the specified file. No trace number is needed or allowed.

NOTE. *Only valid when the spectrum or spectrogram measurements are running.*

Conditions Measurement views: Spectrogram

Group Mass memory commands

Syntax `MMEMory:SGRam:STORe:TRACe <file_name>`

Arguments `<file_name>::=<string>` specifies the file in which to store trace data. The file extension is `.sogram`. You can omit the extension.

Examples `MMEMORY:SGRAM:STORE:TRACE "Spec2"` stores Trace data in the *Spec2.sogram* file.

MMEMory:SPECTrum:LOAD:TRACe (No Query Form)

Loads the spectrum trace data from the specified file.

The parameter `<x>` = 1 to 4; Trace 5 (spectrogram) is invalid.

Conditions Measurement views: Spectrum

Group Mass memory commands

Syntax `MMEMory:SPECTrum:LOAD:TRACe <file_name>`

Arguments `<file_name>::=<string>` specifies the file from which to load trace data. The file extension is `.Specan`. You can omit the extension.

Examples `MMEMORY:SPECTRUM:LOAD:TRACE1 "Sample1"` loads Trace 1 data from the *Sample1.Specan* file.

MMEMory:SPECTrum:SHOW:TRACe<x>

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting “Show recalled trace” in the Recall traces dialog box or selecting Show in the Trace Overview display.

Conditions Measurement views: Spectrum

Group Mass memory commands

Syntax `MMEMory:SPECTrum:SHOW:TRACe<x> { OFF | ON | 0 | 1 }`
`MMEMory:SPECTrum:SHOW:TRACe<x>?`

Related Commands [MMEMory:SPECTrum:LOAD:TRACe](#)

- Arguments** OFF or 0 disables display of the recalled trace.
ON or 1 enables display of the recalled trace.
- Examples** `MMEMory:SPECTRUM:SHOW:TRACe2 ON` enables display of the recalled data loaded in Trace2.

MMEMory:SPECTrum:STORe:TRACe<x> (No Query Form)

Stores the spectrum trace data in the specified file.

The parameter <x> = 1 to 5; All traces are valid.

NOTE. *TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.*

- Conditions** Measurement views: Spectrum
- Group** Mass memory commands
- Syntax** `MMEMory:SPECTrum:STORe:TRACe<x> <file_name>`
- Arguments** `<file_name>::=<string>` specifies the file in which to store trace data. The file extension is .Specan. You can omit the extension.
- Examples** `MMEMory:SPECTRUM:STORe:TRACe1 "Sample1"` stores Trace 1 data in the *Sample1.Specan* file.

MMEMory:SPURious:LOAD:TABLE (No Query Form)

Loads the spurious table containing the limits for enabled ranges from the specified file.

- Conditions** Measurement views: Spurious
- Group** Mass memory commands
- Syntax** `MMEMory:SPURious:LOAD:TABLE <file_name>`

Arguments `<file_name>::=<string>` specifies the file to load the spurious table from. The file extension is `.csv`. You can omit the extension.

Examples `MMEMORY:SPURIOUS:LOAD:TRACE1 "Table1"` loads the spurious table from the `Table1.csv` file.

MMEMory:SPURious:STORE:TABLE (No Query Form)

Stores the spurious table containing the limits for enabled ranges in a specified file in the CSV (Comma Separated Values) format, allowing you to export the file into Microsoft Excel or other database systems.

Conditions Measurement views: Spurious

Group Mass memory commands

Syntax `MMEMory:SPURious:STORE:TABLE <file_name>`

Arguments `<file_name>::=<string>` specifies the file to store the spurious table in. The file extension is `.csv`. You can omit the extension.

Examples `MMEMORY:SPURIOUS:STORE:TABLE "Table1"` stores the spurious table in the `Table1.csv` file.

MMEMory:STORE:IQ (No Query Form)

Saves time-domain IQ waveform in the acquisition memory to a specified file.

Conditions Measurement views: All

Group Mass memory commands

Syntax `MMEMory:STORE:IQ <file_name>`

Arguments `<file_name>::=<string>` specifies the file to save IQ data. The file extension is `.tiq`. You can omit the extension.

Examples `MMEMORY:STORE:IQ "IQ1"` saves IQ data to the *IQ1.tiq* file.

MMEMory:STORE:IQ:CSV (No Query Form)

Saves time-domain IQ waveform in the acquisition memory to a specified file in the CSV (Comma Separated Values) format, allowing you to export the file into Microsoft Excel or other database systems.

Conditions Measurement views: All

Group Mass memory commands

Syntax `MMEMory:STORE:IQ:CSV <file_name>`

Arguments `<file_name>::=<string>` specifies the file to save IQ data.
The file extension is `.csv`. You can omit the extension.

Examples `MMEMORY:STORE:IQ:CSV "IQ2"` saves IQ data to the *IQ2.cs(less t eq)* file.

MMEMory:STORE:IQ:MAT (No Query Form)

Saves time-domain IQ waveform in the acquisition memory to a specified file in the MATLAB format, allowing you to export the file into the MATLAB technical computing environment.

Conditions Measurement views: All

Group Mass memory commands

Syntax `MMEMory:STORE:IQ:MAT <file_name>`

Arguments `<file_name>::=<string>` specifies the file to save IQ data.
The file extension is `.mat`. You can omit the extension.

Examples `MMEMORY:STORE:IQ:MAT "IQ3"` saves IQ data to the *IQ3.mat* file.

MMEMory:STORe:IQ:SELEct:FRAMes

Sets or queries which frames are saved when saving TIQ acquisition data files.

Conditions	Measurement views
Group	Mass memory commands
Syntax	MMEMory:STORe:IQ:SELEct:FRAMes { ACQuisition HISTory SELEcted ALL }
Arguments	<p>ACQuisition saves the entire acquisition that contains the current frame.</p> <p>HISTory saves the current frame.</p> <p>SELEcted saves only selected frames.</p> <p>ALL saves all acquired frames.</p>

MMEMory:STORe:IQ:SELEct:LENGth

Sets or queries what portion of each record is saved when saving acquisition data.

Conditions	Measurement views
Group	Mass memory commands
Syntax	MMEMory:STORe:IQ:SELEct:LENGth { ENTire LENGth } MMEMory:STORe:IQ:SELEct:LENGth?
Arguments	<p>ENTire saves the entire record</p> <p>LENGth saves the portion of the record being analyzed.</p>

MMEMory:STORe:MStAtE (No Query Form)

Stores the measurement parameters to a specified file in the ASCII text format for the currently selected view, allowing you to export the file into other applications.

Conditions	Measurement views: All
-------------------	------------------------

Group	Mass memory commands
Syntax	<code>MMEmory:StORe:MSState <file_name></code>
Arguments	<code><file_name>::=<string></code> specifies the file to store the measurement parameters. The file extension is <code>.txt</code> . You can omit the extension.
Examples	<code>MMEmORY:StORe:MSState "MSTATE1"</code> stores the measurement parameters to the <code>MSTATE1.txt</code> file.

MMEmory:StORe:RESults (No Query Form)

Stores the measurement results including measurement parameters and trace data to a specified file in the CSV (Comma Separated Values) format for the currently selected view, allowing you to export the file into Microsoft Excel or other database systems.

Conditions	Measurement views: All
Group	Mass memory commands
Syntax	<code>MMEmory:StORe:RESults <file_name></code>
Arguments	<code><file_name>::=<string></code> specifies the file to store the measurement results. The file extension is <code>.csv</code> . You can omit the extension.
Examples	<code>MMEmORY:StORe:RESults "RESULT1"</code> stores the measurement results to the <code>RESULT1.csv</code> file.

MMEmory:StORe:SCReen (No Query Form)

Stores the current display as a bitmap image file in one of several standard formats. When no format is specified, the system uses the default, `.png`.

Conditions	Measurement views: All
Group	Mass memory commands

Syntax `MMEemory:STORE:SCREen <file_name>{ .bmp | .jpg | .png }`

Arguments `<file_name>::=<string>` specifies the file to store the screen image.

Examples `MMEemory:STORE:SCREen "RESULT1.png"` stores the current screen image into the file *RESULT1.png*.

MMEemory:STORE:STATE (No Query Form)

Stores the instrument setup to a specified file for the currently selected view.

Conditions Measurement views: All

Group Mass memory commands

Syntax `MMEemory:STORE:STATE <file_name>`

Arguments `<file_name>::=<string>` specifies the file to store the instrument setup. The file extension is `.setup`. You can omit the extension.

Examples `MMEemory:STORE:STATE "STATE1"` stores the instrument setup in the *STATE1.setup* file.

MMEemory:STORE:TRACe (No Query Form)

Stores the trace data in a specified file for the currently selected view.

Conditions Measurement views (See Table 2-34 on page 2-510.)

Group Mass memory commands

Syntax `MMEemory:STORE:TRACe <file_name>`

Related Commands [MMEemory:IQVTIME:SHOW:TRACe:I](#)

- Arguments** <file_name>::=<string> specifies the file to store the trace data in. The file extension is named for the measurement view as shown in the table (See Table 2-34.) The trace file is not available in some views which are indicated by "NA" in the file extension column. For the views that allow multiple-trace display, select the trace to load or store using the command listed in the trace selection column.
- Examples** `MMEMORY:STORE:TRACE "TRACE1"` stores the trace data in the *TRACE1.Specan* file when the spectrum view is selected.

MMEMory:TOVerview:LOAD:TRACe1 (No Query Form)

Loads the trace data from a specified file into Trace1. Refer to (See Table 2-34.) for the correct file extensions for each trace type.

- Conditions** Measurement views
- Group** Mass memory commands
- Syntax** `MMEMory:TOVerview:LOAD:TRACe1 <file_name>`

Related Commands [MMEMory:STORe:TRACe](#)

- Arguments** <file_name>::=<string> specifies the file path and name to load the trace data from. The file extension is named for the measurement view.(See Table 2-34.). Most trace file types are compatible with only one Measurement view.
- Examples** `MMEMory:TOVerview:LOAD:TRACe1 "TRIALB"` loads the trace data from the file *TRIALB.TOV* when the spectrum view is selected.

MMEMory:TOVerview:SHOW:TRACe1

Enables display of a recalled trace file in Trace<x>. The result is the same as selecting "Show recalled trace" in the Recall traces dialog box or selecting Show in the Trace Overview display.

- Conditions** Measurement views

Group	Mass memory commands
Syntax	<code>MMEMemory:TOVerview:SHOW:TRACe1 { OFF ON 0 1 }</code> <code>MMEMemory:TOVerview:SHOW:TRACe1?</code>
Related Commands	MMEMemory:TOVerview:LOAD:TRACe1
Arguments	OFF or 0 disables display of the recalled trace. ON or 1 enables display of the recalled trace.
Examples	<code>MMEMemory:TOVerview:SHOW:TRACe1 ON</code> enables display of the recalled data loaded in Trace2.

MMEMemory:TOVerview:STORE:TRACe1 (No Query Form)

Stores the trace data for Trace1 into the specified file.

Conditions	Measurement views
Group	Mass memory commands
Syntax	<code>MMEMemory:TOVerview:STORE:TRACe1 <file_name></code>
Related Commands	MMEMemory:STORE:TRACe
Arguments	<code><file_name>::=<string></code> specifies the file to store the trace data in. The file extension is named for the measurement view as shown in the table (See Table 2-34.) The trace file is not available in some views which are indicated by "NA" in the file extension column. For the views that allow multiple-trace display, select the trace to load or store using the command listed in the trace selection column.
Examples	<code>MMEMemory:TOVerview:STORE:TRACe1 "TriAlB"</code> stores the Trace1 data into the file <i>TRIALB.TOV</i> when a spectrum view is selected.

***OPC**

Generates the operation complete message in the Standard Event Status Register (SESR) when all pending operations finish. The *OPC? query places the ASCII character "1" into the output queue when all pending operations are finished. The *OPC? response is not available to read until all pending operations finish.

The *OPC command allows you to synchronize the operation of the analyzer with your application program. Refer to *Synchronizing Execution*(See page 3-12.) for the details.

Conditions Measurement views: All

Group IEEE common commands

Syntax *OPC
*OPC?

Arguments None

***OPT? (Query Only)**

Returns a list of options installed in your analyzer.

Conditions Measurement views: All

Group IEEE common commands

Syntax *OPT?

Arguments None

Returns The numbers of all the options installed in the analyzer, separated by commas. If no options have been installed, 0 is returned. The following table lists the options for the RSA6100A Series analyzers.

Table 2-35: Instrument options

Option	Description
01	Internal preamp, 5 MHz - 3 GHz, 30 dB gain, 8 dB noise figure at 2 GHz, typical

Table 2-35: Instrument options (cont.)

Option	Description
02	256 Msample deep memory, frequency mask trigger
05	Digital IQ output and 500 MHz analog IF output
06 ¹	Removable HDD, 80 GB
07 ¹	DVD-RW
20	Advanced signal analysis (including pulse measurements)
21	General purpose modulation analysis
110	110 MHz real-time capture bandwidth
1R ¹	Rackmount

¹ These options are not returned from this query.

Examples *OPT? might return 02 , 05 , 21, indicating that Option 02, 05, and 21 are currently installed in the analyzer.

OUTPut:IF:{BANDwidth|BWIDth}

Sets or queries the IF output filter when [OUTPut:IF\[:STATe\]](#) is set to ON.

Conditions Measurement views: All (Option 05 only)

Group Output commands

Syntax OUTPut:IF:{BANDwidth|BWIDth} { FLATtop | GAUSSian }
OUTPut:IF:{BANDwidth|BWIDth}?

Arguments FLATtop selects the flattop filter.
GAUSSian selects the Gaussian filter.

Examples OUTPUT:IF:BANDWIDTH GAUSSian selects the Gaussian filter for the IF output.

OUTPut:IF[:STATe]

Determines whether to turn on or off the 500 MHz IF Out on the rear panel.

Conditions Measurement views: All (Option 05 only)

Group	Output commands
Syntax	OUTPut:IF[:STATe] { OFF ON 0 1 } OUTPut:IF[:STATe]?
Related Commands	OUTPut:IF:{BANDwidth BWIDth}
Arguments	OFF or 0 turns off IF Out. ON or 1 turns on IF Out.
Examples	OUTPUT:IF:STATE ON turns on IF Out.

OUTPut:IQ[:STATe]

Determines whether to enable or disable the digital IQ output data stream from the rear panel connectors.

Conditions	Measurement views: All (Option 05 only)
Group	Output commands
Syntax	OUTPut:IQ[:STATe] { 0 1 OFF ON } OUTPut:IQ[:STATe]?
Arguments	OFF or 0 disables the digital IQ output. ON or 1 enables the digital IQ output. At *RST, this value is set to OFF.
Examples	OUTPUT:IQ:STATE ON enables the digital IQ output.

OUTPut:NOISe[:STATe]

Determines whether to turn on or off the +28 V DC Out on the rear panel.

Conditions	Measurement views: All
-------------------	------------------------

Group	Output commands
Syntax	OUTPUT:NOISE[:STATE] { OFF ON 0 1 } OUTPUT:NOISE[:STATE]?
Arguments	OFF or 0 turns off +28 V DC Out. ON or 1 turns on +28 V DC Out.
Examples	OUTPUT:NOISE:STATE ON turns on +28 V DC Out.

READ:ACPower? (Query Only)

Returns the Channel power and ACPR measurement results for all available channels.

Conditions	Measurement views: Channel power and ACPR
Group	Read commands
Syntax	READ:ACPower?
Arguments	None
Returns	<p><chan_power>, <acpr_lower(1)>, <acpr_upper(1)>, <acpr_lower(2)>, <acpr_upper(2)>, ... <acpr_lower(n)>, <acpr_upper(n)></p> <p>Where <chan_power> is the average power of the main channel as the power reference in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command. <acpr_lower(n)> is the ACPR for the lower channel #n in dB. <acpr_upper(n)> is the ACPR for the upper channel #n in dB.</p> <p>The number of n depends on the setting of the [SENSe]:ACPower:CHANnel:PAIRs command.</p>
Examples	<p>READ:ACPOWER? might return 4.227, -28.420, -23.847, -22.316, -29.225, indicating (average power of the main channel) = 4.227 dBm, (ACPR for the lower channel 1) = -28.420 dB,</p>

(ACPR for the upper channel 1) = -23.847 dB,
(ACPR for the lower channel 2) = -22.316 dB, and
(ACPR for the upper channel 2) = -29.225 dB.

READ:ACPower:CHANnel:POWer? (Query Only)

Returns the average power of the main channel (power reference) in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Read commands

Syntax READ:ACPower:CHANnel:POWer?

Arguments None

Returns <chan_power> := <NRf> is the average power of the main channel in dBm. The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples READ:ACPOWER:CHANNEL:POWER? might return 4.227, indicating that the average power of the main channel is 4.227 dBm.

READ:ACPower:SPECtrum? (Query Only)

Returns spectrum trace data of the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Read commands

Syntax READ:ACPower:SPECtrum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the spectrum trace data in dBm for the point n, 4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `READ:ACPOWER:SPECTRUM?` might return `#43204xxxx...` (3204-byte data) for the spectrum trace data of the Channel power and ACPR measurement.

READ:{AM|FM|PM}? (Query Only)

Returns the trace data in the AM/FM/PM measurement.

Conditions Measurement views: AM, FM, PM

Group Read commands

Syntax `READ:{AM|FM|PM}?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the modulation factor in percent (AM), frequency deviation in Hz (FM), or phase deviation in degrees (PM) at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `READ:AM` might return `#3156xxxx...` (156-byte data) for the AM measurement trace.

READ:AM:AMINdex? (Query Only)

Returns the modulation index which is (positive peak modulation factor - negative peak modulation factor)/2, returned as a percentage (%).

Conditions Measurement views: AM

Group	Read commands
Syntax	READ:AM:AMINDEX?
Arguments	None
Returns	<value> ::= <NRf> the modulation index.
Examples	READ:AM:AMINDEX? might return 36.48, indicating the modulation index is 36.48%.

READ:AM:AMNegative? (Query Only)

Returns the negative peak modulation factor (-AM) in the AM measurement.

Conditions	Measurement views: AM
Group	Read commands
Syntax	READ:AM:AMNegative?
Arguments	None
Returns	<-AM> ::= <NRf> is the negative peak modulation factor in percent (%).
Examples	READ:AM:AMNEGATIVE? might return -23.4, indicating the negative peak modulation factor is -23.4%.

READ:AM:AMPositive? (Query Only)

Returns the positive peak modulation factor (+AM) in the AM measurement.

Conditions	Measurement views: AM
Group	Read commands

Syntax READ:AM:AMPositive?

Arguments None

Returns <+AM>::=<NRF> is the positive peak modulation factor in percent (%).

Examples READ:AM:AMPOSITIVE? might return 43.8, indicating the positive peak modulation factor is 43.8%.

READ:AM:RESult? (Query Only)

Returns the AM measurement results.

Conditions Measurement views: AM

Group Read commands

Syntax READ:AM:RESult?

Arguments None

Returns <+AM>, <-AM>, <Total AM>

Where

<+AM>::=<NRF> is the positive peak modulation factor in percent (%).

<-AM>::=<NRF> is the negative peak modulation factor in percent (%).

<Total AM>::=<NRF> is the (peak to peak modulation factor)/2 in percent (%).

Examples READ:AM:RESULT? might return 62.63, -50.89, 56.76.

READ:AVTime:AVERage? (Query Only)

Returns the RMS (root-mean-square) value for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions Measurement views: Amplitude versus Time

Group	Read commands
Syntax	READ:AVTime:AVERAge?
Arguments	None
Returns	<avg> ::= <Nrf> is the RMS amplitude in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	READ:AVTIME:AVERAGE? might return -2.53, indicating the RMS amplitude is -2.53 dBm.

READ:AVTime:{FIRSt|SECOnd|THIRd|FOURth}? (Query Only)

Returns the trace data in the Amplitude versus Time measurement.

The mnemonics FIRSt, SECOnd, THIRd, and FOURth represent Trace 1, Trace 2, Trace 3, and Math trace, respectively. The traces can be specified by the TRACe<x>:AVTime command subgroup.

Conditions	Measurement views: Amplitude versus Time
Group	Read commands
Syntax	READ:AVTime:{FIRSt SECOnd THIRd FOURth}?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude in dBm at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	READ:AVTIME:FIRST? might return #3156xxxx... (156-byte data) for Trace 1.

READ:AVTime:MAXimum? (Query Only)

Returns the maximum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions	Measurement views: Amplitude versus Time
Group	Read commands
Syntax	READ:AVTime:MAXimum?
Related Commands	READ:AVTime:MAXLocation?
Arguments	None
Returns	<max>::=<Nrf> is the maximum Amplitude in dBm. The unit can be changed by the [SENSE]:POWER:UNITs command.
Examples	READ:AVTIME:MAXIMUM? might return -2.84, indicating the maximum amplitude is -2.84 dBm.

READ:AVTime:MAXLocation? (Query Only)

Returns the time at which the amplitude is maximum for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions	Measurement views: Amplitude versus Time
Group	Read commands
Syntax	READ:AVTime:MAXLocation?
Related Commands	READ:AVTime:MAXimum?
Arguments	None

Returns <max_time>::=<NRf> is the time at the maximum in seconds.

Examples READ:AVTIME:MAXLOCATION? might return 25.03E-9, indicating the amplitude is maximum at 25.03 ns.

READ:AVTime:MINimum? (Query Only)

Returns the minimum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions Measurement views: Amplitude versus Time

Group Read commands

Syntax READ:AVTime:MINimum?

Related Commands [READ:AVTime:MINLocation?](#)

Arguments None

Returns <min>::=<NRf> is the minimum amplitude in dBm.
The unit can be changed by the [\[SENSE\]:POWER:UNITs](#) command.

Examples READ:AVTIME:MINIMUM? might return -57.64, indicating the minimum amplitude is -57.64 dBm.

READ:AVTime:MINLocation? (Query Only)

Returns the time at which the amplitude is minimum for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions Measurement views: Amplitude versus Time

Group Read commands

Syntax READ:AVTime:MINLocation?

Related Commands	READ:AVTime:MINimum?
Arguments	None
Returns	<code><min_time>::=<NRf></code> is the time at the minimum in seconds.
Examples	<code>READ:AVTIME:MINLOCATION?</code> might return <code>450.7E-9</code> , indicating the amplitude is minimum at 450.7 ns.

READ:AVTime:RESult? (Query Only)

Returns the measurement results for the selected trace in the Amplitude versus Time measurement. Select the trace using the [TRACe<x>:AVTime:SElect](#) command.

Conditions	Measurement views: Amplitude versus Time
Group	Read commands
Syntax	<code>READ:AVTime:RESult?</code>
Arguments	None
Returns	<code><max>, <max_time>, <min>, <min_time>, <rms></code> Where <code><max>::=<NRf></code> is the maximum amplitude in dBm. <code><max_time>::=<NRf></code> is the time at the maximum in seconds. <code><min>::=<NRf></code> is the minimum amplitude in dBm. <code><min_time>::=<NRf></code> is the time at the minimum in seconds. <code><rms>::=<NRf></code> is the RMS amplitude in dBm. The unit of amplitude can be changed by the [SENSE]:POWER:UNITs command.
Examples	<code>READ:AVTIME:RESULT?</code> might return <code>-2.68, 48.62E-6, -82.47, 22.11E-6, -8.24</code> , indicating that the maximum amplitude is -2.68 dBm at 48.62 μ s, the minimum amplitude is -82.47 dBm at 22.11 μ s, and the RMS amplitude is -8.24 dBm.

READ:CCDF? (Query Only)

Returns the CCDF measurement results.

Conditions	Measurement views: CCDF
Group	Read commands
Syntax	READ:CCDF?
Arguments	None
Returns	<p><avg_amp1>, <avg_ccdf>, <crest_factor>, <amp1_10>, <amp1_1>, <amp1_p1>, <amp1_p01>, <amp1_p001>, <amp1_p0001></p> <p>Where</p> <p><avg_amp1> is the average amplitude in dBm. The unit can be changed by the [SENSe]:POWER:UNITs command.</p> <p><avg_ccdf> is the average CCDF in percent.</p> <p><crest_factor> is the crest factor in dB.</p> <p><amp1_10> is the amplitude at CCDF of 10% in dB.</p> <p><amp1_1> is the amplitude at CCDF of 1% in dB.</p> <p><amp1_p1> is the amplitude at CCDF of 0.1% in dB.</p> <p><amp1_p01> is the amplitude at CCDF of 0.01% in dB.</p> <p><amp1_p001> is the amplitude at CCDF of 0.001% in dB.</p> <p><amp1_p0001> is the amplitude at CCDF of 0.0001% in dB.</p>
Examples	<p>READ:CCDF? might return</p> <p>-33.35, 35.8, 9.75, 3.88, 7.07, 8.50, 9.25, 9.72, 9.74, indicating</p> <p>(average amplitude) = -33.35 dBm,</p> <p>(average CCDF) = 35.8%,</p> <p>(crest factor) = 9.75 dB,</p> <p>(amplitude at CCDF of 10%) = 3.88 dB,</p> <p>(amplitude at CCDF of 1%) = 7.07 dB,</p> <p>(amplitude at CCDF of 0.1%) = 8.50 dB,</p> <p>(amplitude at CCDF of 0.01%) = 9.25 dB,</p> <p>(amplitude at CCDF of 0.001%) = 9.72 dB, and</p> <p>(amplitude at CCDF of 0.0001%) = 9.74 dB.</p>

READ:CCDF:{FIRST|SECond|THIRd}:X? (Query Only)

Returns the horizontal values of the specified trace in the CCDF measurement.

The mnemonics FIRSt, SECond, and THIRd represent Trace 1, Trace 2, and Gaussian reference curve, respectively.

NOTE. This query is invalid when *[SENSe]:CCDF:TIME:TYPE* is set to *CONTinuous* or *TOTal*.

Conditions	Measurement views: CCDF
Group	Read commands
Syntax	READ:CCDF:{FIRSt SECond THIRd}:X?
Related Commands	READ:CCDF:{FIRSt SECond THIRd}[:Y]?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><x(2)>...<x(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)> is the horizontal value (dB) of the CCDF graph at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	READ:CCDF:FIRSt:X might return #41024xxxx... (1024-byte data) for the horizontal values of Trace 1.

READ:CCDF:{FIRSt|SECond|THIRd}:XY? (Query Only)

Returns the horizontal and vertical value pairs of the specified trace in the CCDF measurement.

The mnemonics FIRSt, SECond, and THIRd represent Trace 1, Trace 2, and Gaussian reference curve, respectively.

NOTE. This query is invalid when *[SENSe]:CCDF:TIME:TYPE* is set to *CONTinuous* or *TOTal*.

Conditions	Measurement views: CCDF
-------------------	-------------------------

Group	Read commands
Syntax	READ:CCDF:{FIRSt SECond THIRd}:XY?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)>...<x(n)><y(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)><y(n)> is the horizontal value (dB) and vertical value (%) pair at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	READ:CCDF:FIRSt:XY? might return #41024xxxx... (1024-byte data) for the horizontal and vertical value pairs of Trace 1.

READ:CCDF:{FIRSt|SECond|THIRd}[:Y]? (Query Only)

Returns the vertical values of the specified trace in the CCDF measurement.

The mnemonics FIRSt, SECond, and THIRd represent Trace 1, Trace 2, and Gaussian reference curve, respectively.

NOTE. This query is invalid when *[SENSe]:CCDF:TIME:TYPE* is set to *CONTinuous* or *TOTal*.

Conditions	Measurement views: CCDF
Group	Read commands
Syntax	READ:CCDF:{FIRSt SECond THIRd}[:Y]?
Arguments	None
Returns	#<num_digit><num_byte><y(1)><y(2)>...<y(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow.

<y(n)> is the vertical value (%) of the CCDF graph at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:CCDF:FIRST:Y might return #41024xxxx... (1024-byte data) for the vertical values of Trace 1.

READ:CONStE:FERRor? (Query Only)

Returns the frequency error in Hz. The frequency error is the difference between the measured carrier frequency of the signal and the user-selected center frequency of the analyzer.

Group Read commands

Syntax READ:CONStE:FERRor?

Related Commands [READ:EVM:FERRor?](#)

Arguments None.

Returns <freq_error>::=<Nrf> which is the frequency error in Hz.

Examples READ:CONStE:FERRor? might return -10.7E+3, which is a frequency error of -10.7 kHz.

READ:CONStE:RESuLts? (Query Only)

Returns the constellation measurement results of EVM RMS, peak and location displayed on the bottom of the screen.

Conditions Measurement views: Constellation

Group Read commands

Syntax READ:CONStE:RESuLts?

Arguments None

- Returns** For modulation types 2|4|8|16FSK or C4FM:
 FSK_deviation_Avg_Leftmost, FSK_deviation_Avg_Rightmost
 Where
 FSK_deviation_Avg_Leftmost is the average FSK deviation of the left-most symbol in Hz.
 FSK_deviation_Avg_Rightmost is the average FSK deviation of the right-most symbol in Hz.
 For all other valid modulation types:
 <EVM_RMS>, <EVM_peak>, <location>
 Where
 <EVM_RMS> ::= <NRf> is the RMS EVM in percent (%).
 <EVM_peak> ::= <NRf> is the peak EVM in percent (%).
 <location> ::= <NRf> is the peak location in symbol number.
 The time unit can be changed by the [\[SENSE\]:DDEMod:TIME:UNITS](#) command.
- Examples** READ:CONStE:RESUlTS? might return 2.841, 3.227, 68.000, indicating that the RMS EVM is 2.841% and the peak EVM is 3.227% at symbol #68.

READ:CONStE:TRACe? (Query Only)

Returns the constellation trace data.

- Conditions** Measurement views: Constellation
- Group** Read commands
- Syntax** READ:CONStE:TRACe?
- Arguments** None
- Returns** #<num_digit><num_byte><I(1)><Q(1)><I(2)><Q(2)>...<I(n)><Q(n)>
 Where
 <num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <I(n)> and <Q(n)> are the normalized I- and Q-coordinate values at the nth data point. 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:CONSTE:TRACE? might return #43848xxxx... (3848-byte data) for the constellation trace data.

READ:DDEMod:STABLE? (Query Only)

Returns the symbol table data.

Conditions Measurement views: Symbol table

Group Read commands

Syntax READ:DDEMod:STABLE?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the symbol table data for the point n,

\4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:DDEMOD:STABLE? might return #3512xxxx... (512-byte data) for the symbol table.

READ:DIQVtime:FERRor? (Query Only)

Returns the frequency error in the Demod I&Q versus Time measurement.

Conditions Measurement views: Demod I&Q versus Time

Group Read commands

Syntax READ:DIQVtime:FERRor?

Arguments None

Returns <freq_error>::=<NRF> is the frequency error in Hz.

Examples READ:DIQVTIME:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:DIQVtime:I? (Query Only)

Returns the I versus Time trace data.

Conditions Measurement views: Demod I&Q versus Time

Group Read commands

Syntax READ:DIQVtime:I?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the I level in volts at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:DIQVTIME:I? might return #3160xxxx... (160-byte data) for the I versus Time trace.

READ:DIQVtime:Q? (Query Only)

Returns the Q versus Time trace data.

Conditions Measurement views: Demod I&Q versus Time

Group Read commands

Syntax READ:DIQVtime:Q?

Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the Q level in volts at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	READ:DIQVTIME:Q? might return #3160xxxx... (160-byte data) for the Q versus Time trace.

READ:DPSA:RESuLts:TRACe<x>? (Query Only)

Acquires a waveform and then returns waveform data of the specified trace <x> in the DPX spectrum measurement, where x is 1 to 5. The traces 1–4 are in the standard form. Trace 5 is the bitmap trace and its data is returned in a binary block.

Conditions	Measurement views: DPX spectrum
Group	Read commands
Syntax	READ:DPSA:RESuLts:TRACe<x>?
Arguments	<NR1>
Returns	For traces 1 to 4: #<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude of the trace sample at the n th data point. <data(n) is in the 4-byte little endian floating-point format specified in IEEE 488.2. For trace 5, the format differs depending on whether Option 200 is installed in the instrument. Without Option 200, the format is a binary block of unsigned 16 bit integers. Each value ranges from 0 to 2 ¹⁶ -1, where 2 ¹⁶ -1 represents 100%.

With Option 200, the format is a binary block of 32 bit floating point values. Each value ranges from 0 to 1.0, where 1.0 represents 100%.

Examples `READ:DPSA:RESULTS:TRACE1?` might return `#42004xxxx...` (2004-byte of data) for the waveform data of trace one (1).

READ:DPSA:TRACE:AVERAGE? (Query Only)

Acquires a waveform and then returns waveform data of the average trace in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Read commands

Syntax `READ:DPSA:TRACE:AVERAGE?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the waveform data of the average trace for the point `n` in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSE\]:POWER:UNITS](#) command.

Examples `READ:DPSA:TRACE:AVERAGE?` might return `#42004xxxx...` (2004-byte data) for the waveform data of the average trace.

READ:DPSA:TRACE:BITMap? (Query Only)

Acquires a waveform and then returns trace waveform data of the bitmap trace in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Read commands

Syntax READ:DPSA:TRACe:BITMap?

Arguments None

Returns For trace 5, the format differs depending on whether Option 200 is installed in the instrument. Without Option 200, the format is a binary block of unsigned 16 bit integers. Each value ranges from 0 to $2^{16}-1$, where $2^{16}-1$ represents 100%.

With Option 200, the format is a binary block of 32 bit floating point values. Each value ranges from 0 to 1.0, where 1.0 represents 100%.

Examples READ:DPSA:TRACE:BITMAP? might return #42004xxxx... (2004-byte data) for the waveform data of the bitmap trace.

READ:DPSA:TRACe:MATH? (Query Only)

Returns waveform data of the math trace in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Read commands

Syntax READ:DPSA:TRACe:MATH?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the waveform data of the math trace for the point n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples READ:DPSA:TRACE:MATH? might return #42004xxxx... (2004-byte data) for the waveform data of the math trace.

READ:DPSA:TRACe:MAXimum? (Query Only)

Returns waveform data of the maximum trace in the DPX spectrum measurement.

Conditions	Measurement views: DPX spectrum
Group	Read commands
Syntax	READ:DPSA:TRACe:MAXimum?
Arguments	None
Returns	<code>#<num_digit><num_byte><data(1)><data(2)>...<data(n)></code> Where <code><num_digit></code> is the number of digits in <code><num_byte></code> . <code><num_byte></code> is the number of bytes of data that follow. <code><data(n)></code> is the waveform data of the maximum trace for the point n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	READ:DPSA:TRACe:MAXIMUM? might return #42004xxxx... (2004-byte data) for the waveform data of the maximum trace.

READ:DPSA:TRACe:MINimum? (Query Only)

Returns waveform data of the minimum trace in the DPX spectrum measurement.

Conditions	Measurement views: DPX spectrum
Group	Read commands
Syntax	READ:DPSA:TRACe:MINimum?
Arguments	None
Returns	<code>#<num_digit><num_byte><data(1)><data(2)>...<data(n)></code> Where

<num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <data(n)> is the waveform data of the minimum trace for the point n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.
 The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `READ:DPSA:TRACE:MINIMUM?` might return `#42004xxxx...` (2004-byte data) for the waveform data of the minimum trace.

READ:EDiagram:FDEVIation? (Query Only)

Returns the frequency deviation versus Time trace data with the X values.

Group Read commands

Syntax `READ:EDIagram:FDEVIation?`

Related Commands

Returns `#<num_digit><num_byte><Y(1)><X(1)><Y(2)><X(2)>...<Y(n)><X(n)>`

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<Y(n)> and <X(n)> is frequency deviation in Hz and time (symbols) pair at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `READ:EDIAGRAM:FDEVIATION?` might return `#3160xxxx...` (160-byte data) for the frequency deviation versus Time trace.

READ:EDiagram:FERRor? (Query Only)

Returns the frequency error in the eye diagram measurement.

Conditions Measurement views: Eye diagram

Group Read commands

Syntax `READ:EDIagram:FERRor?`

Arguments	None
Returns	<freq_error> := <NRF> is the frequency error in Hz.
Examples	READ:EDIAGRAM:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:EDIagram:I? (Query Only)

Returns the I versus Time trace data.

Conditions	Measurement views: Eye diagram
Group	Read commands
Syntax	READ:EDIagram:I?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <Y(n)><X(n)> is the I level (normalized) and time (symbols) pair at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	READ:EDIAGRAM:I? might return #3160xxxx... (160-byte data) for the I versus Time trace.

READ:EDIagram:Q? (Query Only)

Returns the Q versus Time trace data.

Conditions	Measurement views: Eye diagram
Group	Read commands

Syntax READ:EDIagram:Q?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<Y(n)><X(n)> is the Q level (normalized) and time (symbols) pair at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:EDIAGRAM:Q? might return #3160xxxx... (160-byte data) for the Q versus Time trace.

READ:EVM:FERRor? (Query Only)

Returns the frequency error in the EVM versus Time measurement.

Conditions Measurement views: EVM versus Time

Group Read commands

Syntax READ:EVM:FERRor?

Arguments None

Returns <freq_error>::=<Nrf> is the frequency error in Hz.

Examples READ:EVM:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:EVM:PEAK? (Query Only)

Returns the peak value in the EVM versus Time measurement.

Conditions Measurement views: EVM versus Time

Group	Read commands
Syntax	READ:EVM:PEAK?
Related Commands	READ:EVM:PINdex?
Arguments	None
Returns	<peak> ::= <NRf> is the peak EVM value in percent (%).
Examples	READ:EVM:PEAK? might return 1.32, indicating the peak EVM value is 1.32%.

READ:EVM:PINdex? (Query Only)

Returns the time at the EVM peak.

Conditions	Measurement views: EVM versus Time
Group	Read commands
Syntax	READ:EVM:PINdex?
Related Commands	READ:EVM:PEAK?
Arguments	None
Returns	<peak_time> ::= <NRf> is the time at the EVM peak in symbol number. The unit can be changed by the [SENSE]:DDEMod:TIME:UNITS command.
Examples	READ:EVM:PINDEX? might return 68.000, indicating that the EVM peak is at symbol #68.

READ:EVM:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the EVM versus Time measurement.

Conditions	Measurement views: EVM versus Time
Group	Read commands
Syntax	READ:EVM:RMS?
Arguments	None
Returns	<rms>:::=<nrf> is the RMS EVM value in percent (%).
Examples	READ:EVM:RMS? might return 0.582, indicating the RMS EVM value is 0.582%.

READ:EVM:TRACe? (Query Only)

Returns the EVM versus Time trace data.

Conditions	Measurement views: EVM versus Time
Group	Read commands
Syntax	READ:EVM:TRACe?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the EVM versus Time trace data for the point n in percent (%), 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	READ:EVM:TRACe? might return #42036xxxx... (2036-byte data) for the EVM versus Time trace.

READ:FDVTime:FERRor? (Query Only)

Returns the frequency error in the Frequency deviation versus Time measurement.

Conditions Measurement views: Frequency deviation versus Time

Group Read commands

Syntax READ:FDVTime:FERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Examples READ:FDVTime:FERRor? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:FDVTime:TRACe? (Query Only)

Returns the Frequency deviation versus Time trace data.

Conditions Measurement views: Frequency deviation versus Time

Group Read commands

Syntax READ:FDVTime:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the frequency deviation in Hz at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:FDVTIME:TRACE? might return #3160xxxx... (160-byte data) for the Frequency deviation versus Time trace.

READ:{FM|PM}:FERRor? (Query Only)

Returns the frequency error in the Frequency modulation and Phase modulation measurements.

Conditions Measurement views: Frequency and Phase modulation

Group Read commands

Syntax READ:{FM|PM}:FERRor?

Arguments None

Returns <freq_error>::=<Nrf> is the frequency error in Hz.

Examples READ:FM:FERRor? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:FM:PHALf? (Query Only)

Returns the half peak-peak frequency deviation (Pk-Pk/2) in the FM measurement.

Conditions Measurement views: Frequency deviation versus Time

Group Read commands

Syntax READ:FM:PHALf?

Arguments None

Returns <Pk-Pk/2>::=<Nrf> is the half peak-peak frequency deviation in Hz.

Examples READ:FM:PHALF? might return 628.9E+3, indicating the half peak-peak frequency deviation is 628.9 kHz.

READ:FM:PNEGative? (Query Only)

Returns the negative peak frequency deviation ($-Pk$) in the FM measurement.

Conditions Measurement views: FM

Group Read commands

Syntax READ:FM:PNEGative?

Arguments None

Returns $\langle -Pk \rangle ::= \langle NRf \rangle$ is the negative peak frequency deviation in Hz.

Examples READ:FM:PNEGATIVE? might return $-495.6E+3$, indicating the negative peak frequency deviation is -495.6 kHz.

READ:FM:PPOSitive? (Query Only)

Returns the positive peak frequency deviation ($+Pk$) in the FM measurement.

Conditions Measurement views: FM

Group Read commands

Syntax READ:FM:PPOSitive?

Arguments None

Returns $\langle +Pk \rangle ::= \langle NRf \rangle$ is the positive peak frequency deviation in Hz.

Examples READ:FM:PPOSITIVE? might return $763.2E+3$, indicating the positive peak frequency deviation is 763.2 kHz.

READ:FM:PTPeak? (Query Only)

Returns the peak-peak frequency deviation (Pk-Pk) in the FM measurement.

Conditions	Measurement views: FM
Group	Read commands
Syntax	READ:FM:PTPeak?
Arguments	None
Returns	<Pk-Pk>::=<NRf> is the peak-peak frequency deviation in Hz.
Examples	READ:FM:PTPEAK? might return 1.258E+6, indicating the peak-peak frequency deviation is 1.258 MHz.

READ:FM:RESult? (Query Only)

Returns the FM measurement results.

Conditions	Measurement views: FM
Group	Read commands
Syntax	READ:FM:RESult?
Arguments	None
Returns	<+Pk>, <-Pk>, <RMS>, <Pk-Pk>, <Pk-Pk/2> Where <+Pk>::=<NRf> is the positive peak frequency deviation in Hz. <-Pk>::=<NRf> is the negative peak frequency deviation in Hz. <RMS>::=<NRf> is the RMS frequency deviation in Hz. <Pk-Pk>::=<NRf> is the peak-peak frequency deviation in Hz. <Pk-Pk/2>::=<NRf> is the half peak-peak frequency deviation in Hz.

Examples READ:FM:RESULT? might return
763.2E+3,-494.6E+3,271.2E+3,1.258E+6,628.9E+3.

READ:FM:RMS? (Query Only)

Returns the RMS frequency deviation in the FM measurement.

Conditions Measurement views: FM

Group Read commands

Syntax READ:FM:RMS?

Arguments None

Returns <RMS> ::= <NRf> is the RMS frequency deviation in Hz.

Examples READ:FM:RMS? might return 271.2E+3, indicating the RMS frequency deviation is 271.2 kHz.

READ:FVTime? (Query Only)

Returns the Frequency versus Time trace data.

Conditions Measurement views: Frequency versus Time

Group Read commands

Syntax READ:FVTime?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the frequency drift data for the point n in Hz, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:FVTIME? might return #3156xxxx... (156-byte data) for the Frequency versus Time trace.

READ:FVTime:MAXimum? (Query Only)

Returns the maximum value in the Frequency versus Time measurement.

Conditions Measurement views: Frequency versus Time

Group Read commands

Syntax READ:FVTime:MAXimum? imum

Related Commands [READ:FVTime:MAXLocation?](#)

Arguments None

Returns <max>::=<NRF> is the maximum frequency drift in Hz.

Examples READ:FVTIME:MAXIMUM? might return 2.625E+6, indicating the maximum frequency drift is 2.625 MHz.

READ:FVTime:MAXLocation? (Query Only)

Returns the time at which the frequency drift is maximum.

Conditions Measurement views: Frequency versus Time

Group Read commands

Syntax READ:FVTime:MAXLocation?

Related Commands [READ:FVTime:MAXimum?](#)

Arguments	None
Returns	<code><max_time>::=<NRF></code> is the time in seconds at which the frequency drift is maximum.
Examples	<code>READ:FVTIME:MAXLOCATION?</code> might return <code>25.03E-9</code> , indicating the frequency drift is maximum at 25.03 ns.

READ:FVTime:MINimum? (Query Only)

Returns the minimum value in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Read commands
Syntax	<code>READ:FVTime:MINimum?</code>

Related Commands [READ:FVTime:MINLocation?](#)

Arguments	None
Returns	<code><min>::=<NRF></code> is the minimum frequency drift in Hz.
Examples	<code>READ:FVTIME:MINIMUM?</code> might return <code>-6.618E+6</code> , indicating the minimum frequency drift is -6.618 MHz.

READ:FVTime:MINLocation? (Query Only)

Returns the time at which the frequency drift is minimum.

Conditions	Measurement views: Frequency versus Time
Group	Read commands
Syntax	<code>READ:FVTime:MINLocation?</code>

Related Commands	READ:FVTime:MINimum?
Arguments	None
Returns	<code><min_time>::=<NRf></code> is the time in seconds at which the frequency drift is minimum.
Examples	<code>READ:FVTIME:MINLOCATION?</code> might return <code>450.7E-9</code> , indicating the frequency drift is minimum at 450.7 ns.

READ:FVTime:RESult? (Query Only)

Returns the Frequency versus Time measurement results.

Conditions	Measurement views: Frequency versus Time
Group	Read commands
Syntax	<code>READ:FVTime:RESult?</code>
Arguments	None
Returns	<p><code><max>, <max_time>, <min>, <min_time></code></p> <p>Where</p> <p><code><max>::=<NRf></code> is the maximum frequency drift in Hz.</p> <p><code><max_time>::=<NRf></code> is the time in seconds at which the frequency drift is maximum.</p> <p><code><min>::=<NRf></code> is the minimum frequency drift in Hz.</p> <p><code><min_time>::=<NRf></code> is the time in seconds at which the frequency drift is minimum.</p>
Examples	<p><code>READ:FVTIME:RESULT?</code> might return <code>2.625E+6, 25.03E-9, -6.618E+6, 450.7E-9</code>, indicating the maximum frequency drift is 2.625 MHz at 25.03 ns and the minimum frequency drift is -6.618 MHz at 450.7 ns.</p>

READ:IQVTime:I? (Query Only)

Returns the I versus Time trace data.

Conditions Measurement views: RF I&Q versus Time

Group Read commands

Syntax READ:IQVTime:I?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the I level data for the point n in volts, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:IQVTime:I? might return #3160xxxx... (160-byte data) for the I versus Time trace.

READ:IQVTime:MAXimum? (Query Only)

Returns the maximum value in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Read commands

Syntax READ:IQVTime:MAXimum? imum

Related Commands [READ:IQVTime:MAXLocation?](#)

Arguments None

Returns <max>::=<NRf> is the maximum I or Q level in volts.

Examples `READ:IQVTIME:MAXIMUM?` might return 1.214, indicating the maximum I or Q level is 1.214 V.

READ:IQVTime:MAXLocation? (Query Only)

Returns the time at which the I or Q level is maximum.

Conditions Measurement views: RF I&Q versus Time

Group Read commands

Syntax `READ:IQVTime:MAXLocation?`

Related Commands [READ:IQVTime:MAXimum?](#)

Arguments None

Returns `<max_time>::=<NRF>` is the time in seconds at which the I or Q level is maximum.

Examples `READ:IQVTIME:MAXLOCATION?` might return 175.3E-9, indicating the I or Q level is maximum at 175.3 ns.

READ:IQVTime:MINimum? (Query Only)

Returns the minimum value in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Read commands

Syntax `READ:IQVTime:MINimum?`

Related Commands [READ:IQVTime:MINLocation?](#)

Arguments None

Returns <min>::=<Nrf> is the minimum I or Q level in volts.

Examples READ:IQVTime:MINIMUM? might return -370.5E-3, indicating the minimum I or Q level is -370.5 mV.

READ:IQVTime:MINLocation? (Query Only)

Returns the time at which the I or Q level is minimum.

Conditions Measurement views: RF I&Q versus Time

Group Read commands

Syntax READ:IQVTime:MINLocation?

Related Commands [READ:IQVTime:MINimum?](#)

Arguments None

Returns <min_time>::=<Nrf> is the time in seconds at which the I or Q level is minimum.

Examples READ:IQVTime:MINLOCATION? might return 450.7E-9, indicating the I or Q level is minimum at 450.7 ns.

READ:IQVTime:Q? (Query Only)

Returns the Q versus Time trace data.

Conditions Measurement views: IQ versus Time

Group Read commands

Syntax READ:IQVTime:Q?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the Q level data for the point n in volts, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:IQVTIME:Q? might return #3160xxxx... (160-byte data) for the Q versus Time trace.

READ:IQVTime:RESult? (Query Only)

Returns the RF I&Q versus Time measurement results.

Conditions Measurement views: RF I&Q versus Time

Group Read commands

Syntax READ:IQVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>

Where

<max>::=<Nrf> is the maximum I or Q level in volts.

<max_time>::=<Nrf> is the time in seconds at which the I or Q level is maximum.

<min>::=<Nrf> is the minimum I or Q level in volts.

<min_time>::=<Nrf> is the time in seconds at which the I or Q level is minimum.

Examples READ:IQVTIME:RESULT? might return 1.214,175.3E-9,-370.5E-3,450.7E-9, indicating the maximum I or Q level is 1.214 V at 175.3 ns and the minimum I or Q level is -370.5 mV at 450.7 ns.

READ:MCPower:ADJacent:CHANnels? (Query Only)

Returns the power of adjacent channels in order of increasing frequency.

Conditions	Measurement views: MCPR
Group	Read commands
Syntax	READ:MCPower:ADJacent:CHANnelS?
Arguments	None
Returns	<p><acpr_lower(n)>, ... <acpr_lower(2)>, <acpr_lower(1)>, <acpr_upper(1)>, <acpr_upper(2)>, ... <acpr_upper(n)></p> <p>Where <acpr_lower(n)> is the ACPR for the lower channel #n in dB. <acpr_upper(n)> is the ACPR for the upper channel #n in dB.</p> <p>To add a pair of upper and lower adjacent channels, use the [SENSe]:MCPower:CHANnel:ADJacent:ADD command.</p>
Examples	<p>READ:MCPOWER:ADJACENT:CHANNELS? might return -4.420, -4.847, -4.316, -4.225, indicating (ACPR for the lower channel 2) = -4.420 dB, (ACPR for the lower channel 1) = -4.847 dB, (ACPR for the upper channel 1) = -4.316 dB, and (ACPR for the upper channel 2) = -4.225 dB.</p>

READ:MCPower:CHANnel:POWer? (Query Only)

Returns the reference power in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Read commands
Syntax	READ:MCPower:CHANnel:POWer?
Arguments	None
Returns	<p><ref_power>: <NRf> is the reference power in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.</p>

To select the power reference, use the [SENSe]:MCPower:RCHannels commands.

Examples READ:MCPOWER:CHANNEL:POWER? might return 4.227, indicating that the reference power is 4.227 dBm.

READ:MCPower:MAIN:CHANnels? (Query Only)

Returns the power of main channels in order of increasing frequency.

Conditions Measurement views: MCPR

Group Read commands

Syntax READ:MCPower:MAIN:CHANnels?

Related Commands [:SENSe]:MCPower:CHANnel:MAIN commands

Arguments None

Returns <power_main(1)>, <power_main(2)>, ... <power_main(n)>

Where

<power_main(n)> is the power of main channel #n in dBm.

The unit can be changed by the [SENSe]:POWer:UNITs command.

To specify the main channels, use the [SENSe]:MCPower:CHANnel:MAIN commands.

Examples READ:MCPOWER:MAIN:CHANNELS? might return -2.420, -2.847, -2.316, -2.225, indicating (power of the main channel 1) = -2.420 dBm, (power of the main channel 2) = -2.847 dBm, (power of the main channel 3) = -2.316 dBm, and (power of the main channel 4) = -2.225 dBm.

READ:MCPower:SPECTrum? (Query Only)

Returns spectrum trace data of the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Read commands
Syntax	READ:MCPower:SPECTrum?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the spectrum trace data in dBm for the point n, 4-byte little endian floating-point format specified in IEEE 488.2. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	READ:MCPOWER:SPECTRUM? might return #43204xxxx... (3204-byte data) for the spectrum trace data of the MCPR measurement.

READ:MERRor:FERRor? (Query Only)

Returns the frequency error in the Magnitude error versus Time measurement.

Conditions	Measurement views: Magnitude error versus Time
Group	Read commands
Syntax	READ:MERRor:FERRor?
Arguments	None
Returns	<freq_error>::=<NRF> is the frequency error in Hz.
Examples	READ:MERROR:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:MERRor:PEAK? (Query Only)

Returns the peak value in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Read commands

Syntax READ:MERRor:PEAK?

Related Commands [READ:MERRor:PINdex?](#)

Arguments None

Returns <peak>::=<NRf> is the peak magnitude error in percent (%).

Examples READ:MERRor:PEAK? might return 1.57, indicating the peak magnitude error is 1.57%.

READ:MERRor:PINdex? (Query Only)

Returns the time at the magnitude error peak.

Conditions Measurement views: Magnitude error versus Time

Group Read commands

Syntax READ:MERRor:PINdex?

Related Commands [READ:MERRor:PEAK?](#)

Arguments None

Returns <peak_time>::=<NRf> is the time at the magnitude error peak in symbol number. The unit can be changed by the [\[SENSe\]:DDEMod:TIME:UNITs](#) command.

Examples READ:MERROR:PINDEX? might return 68.000, indicating that the magnitude error peak is at symbol #68.

READ:MERRor:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Read commands

Syntax READ:MERRor:RMS?

Arguments None

Returns <rms> ::= <Nrf> is the RMS magnitude error in percent (%).

Examples READ:MERRor:RMS? might return 0.382, indicating the magnitude error is 0.382% RMS.

READ:MERRor:TRACe? (Query Only)

Returns the Magnitude error versus Time trace data.

Conditions Measurement views: Magnitude error versus Time

Group Read commands

Syntax READ:MERRor:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where
<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.
<data(n)> is the magnitude error data for the point n in percent (%),
4-byte little endian floating-point format specified in IEEE 488.2.

Examples `READ:MERROR:TRACE?` might return `#42036xxxx...` (2036-byte data) for the Magnitude error versus Time trace.

READ:OBWidth:FREQuency:ERRor? (Query Only)

Returns the frequency error in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Read commands

Syntax `READ:OBwidth:FREQuency:ERRor?`

Arguments None

Returns <freq_error> ::= <Nrf> is the frequency error in Hz.

Examples `READ:OBWIDTH:FREQUENCY:ERROR?` might return `-10.7E+3`, indicating the frequency error is -10.7 kHz.

READ:OBWidth:OBWidth:BANDwidth? (Query Only)

Returns the occupied bandwidth in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Read commands

Syntax `READ:OBwidth:OBwidth:BANDwidth?`

Arguments None

Returns <OBW> ::= <NRf> is the occupied bandwidth in Hz.

Examples READ:OBWIDTH:OBWIDTH:BANDWIDTH? might return 4.0E+6, indicating the occupied bandwidth is 4 MHz.

READ:OBWidth:OBWidth:LEFT:FREQUENCY? (Query Only)

Returns the left (lower) frequency of the occupied bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Read commands

Syntax READ:OBWidth:OBWidth:LEFT:FREQUENCY?

Related Commands [READ:OBWidth:OBWidth:RIGHT:FREQUENCY?](#)

Arguments None

Returns <OBW_left_freq> ::= <NRf> is the left frequency in Hz.

Examples READ:OBWIDTH:OBWIDTH:LEFT:FREQUENCY? might return 1.498E+9, indicating the left frequency is 1.498 GHz.

READ:OBWidth:OBWidth:LEFT:LEVEL? (Query Only)

Returns the level at the left frequency of the occupied bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Read commands

Syntax READ:OBWidth:OBWidth:LEFT:LEVEL?

Related Commands [READ:OBWidth:OBWidth:RIGHT:LEVEL?](#)

Arguments	None
Returns	<OBW_left_level>::=<Nrf> is the level at the left frequency in dB.
Examples	READ:OBWIDTH:OBWIDTH:LEFT:LEVEL? might return -23.5, indicating the level at the left frequency is -23.5 dB.

READ:OBWidth:OBWidth:POWer? (Query Only)

Returns the reference power in the Occupied Bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Read commands
Syntax	READ:OBWidth:OBWidth:POWer?
Arguments	None
Returns	<OBW_ref_power>::=<Nrf> is the reference power in dBm. The unit can be changed by the [SENSE]:POWer:UNITs command.
Examples	READ:OBWIDTH:OBWIDTH:POWER? might return -10.0, indicating the reference power is -10 dBm.

READ:OBWidth:OBWidth:RIGHT:FREQuency? (Query Only)

Returns the right (higher) frequency of the occupied bandwidth.

Conditions	Measurement views: Occupied Bandwidth
Group	Read commands
Syntax	READ:OBWidth:OBWidth:RIGHT:FREQuency?
Related Commands	READ:OBWidth:OBWidth:LEFT:FREQuency?

Arguments	None
Returns	<OBW_right_freq>::=<Nrf> is the right frequency in Hz.
Examples	READ:OBWIDTH:OBWIDTH:RIGHT:FREQUENCY? might return 1.502E+9, indicating the right frequency is 1.502 GHz.

READ:OBWidth:OBWidth:RIGHT:LEVel? (Query Only)

Returns the level at the right frequency of the occupied bandwidth.

Conditions	Measurement views: Occupied Bandwidth
Group	Read commands
Syntax	READ:OBWidth:OBWidth:RIGHT:LEVel?

Related Commands [READ:OBWidth:OBWidth:LEFT:LEVel?](#)

Arguments	None
Returns	<OBW_right_level>::=<Nrf> is the level at the right frequency in dB.
Examples	READ:OBWIDTH:OBWIDTH:RIGHT:LEVEL? might return -23.5, indicating the level at the right frequency is -23.5 dB.

READ:OBWidth:SPECTrum? (Query Only)

Returns spectrum trace data of the Occupied Bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Read commands
Syntax	READ:OBWidth:SPECTrum?

Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude in dBm at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2. The unit can be changed by the [SENSE]:POWER:UNITS command.
Examples	READ:OBWIDTH:SPECTRUM? might return #43204xxxx... (3204-byte data) for the spectrum trace data of the Occupied Bandwidth measurement.

READ:OBWidth:XDBBandwidth:BANDwidth? (Query Only)

Returns the x dB bandwidth in the Occupied Bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Read commands
Syntax	READ:OBwidth:XDBBandwidth:BANDwidth?
Arguments	None
Returns	<xdbbw>::=<Nrf> is the x dB bandwidth in Hz.
Examples	READ:OBWIDTH:XDBBANDWIDTH:BANDWIDTH? might return 2.0E+6, indicating the x dB bandwidth is 2 MHz.

READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY? (Query Only)

Returns the left (lower) frequency of the x dB bandwidth.

Conditions	Measurement views: Occupied Bandwidth
Group	Read commands

Syntax `READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY?`

Related Commands [READ:OBWidth:XDBBandwidth:RIGHT:FREQUENCY?](#)

Arguments None

Returns `<xdBW_left_freq>::=<Nrf>` is the left frequency in Hz.

Examples `READ:OBWIDTH:XDBBANDWIDTH:LEFT:FREQUENCY?` might return `1.498E+9`, indicating the left frequency is 1.498 GHz.

READ:OBWidth:XDBBandwidth:LEFT:LEVEL? (Query Only)

Returns the level at the left frequency of the x dB bandwidth.

Conditions Measurement views: Occupied Bandwidth

Group Read commands

Syntax `READ:OBWidth:XDBBandwidth:LEFT:LEVEL?`

Related Commands [READ:OBWidth:XDBBandwidth:RIGHT:LEVEL?](#)

Arguments None

Returns `<xdBW_left_level>::=<Nrf>` is the level at the left frequency in dB.

Examples `READ:OBWIDTH:XDBBANDWIDTH:LEFT:LEVEL?` might return `-23.5`, indicating the level at the left frequency is -23.5 dB.

READ:OBWidth:XDBBandwidth:POWER? (Query Only)

Returns the reference power in the x dB bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group	Read commands
Syntax	READ:OBwidth:XDBBandwidth:POWER?
Arguments	None
Returns	<xdbbw_ref_power>::=<Nrf> is the reference power in dBm. The unit can be changed by the [SENSE]:POWER:UNITs command.
Examples	READ:OBWIDTH:XDBBANDWIDTH:POWER? might return -10.0, indicating the reference power is -10 dBm.

READ:OBWidth:XDBBandwidth:RIGHT:FREQUENCY? (Query Only)

Returns the right (higher) frequency of the x dB bandwidth.

Conditions	Measurement views: Occupied Bandwidth
Group	Read commands
Syntax	READ:OBwidth:XDBBandwidth:RIGHT:FREQUENCY?
Related Commands	READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY?
Arguments	None
Returns	<xdbbw_right_freq>::=<Nrf> is the right frequency in Hz.
Examples	READ:OBWIDTH:XDBBANDWIDTH:RIGHT:FREQUENCY? might return 1.502E+9, indicating the right frequency is 1.502 GHz.

READ:OBWidth:XDBBandwidth:RIGHT:LEVEL? (Query Only)

Returns the level at the right frequency of the x dB bandwidth.

Conditions	Measurement views: Occupied Bandwidth
-------------------	---------------------------------------

Group	Read commands
Syntax	READ:OBWidth:XDBBandwidth:RIGHT:LEVEL?
Related Commands	READ:OBWidth:XDBBandwidth:LEFT:LEVEL?
Arguments	None
Returns	<xdbbw_right_level>::=<Nrf> is the level at the right frequency in dB.
Examples	READ:OBWIDTH:XDBBANDWIDTH:RIGHT:LEVEL? might return -23.5, indicating the level at the right frequency is -23.5 dB.

READ:PERRor:FERRor? (Query Only)

Returns the frequency error in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Read commands
Syntax	READ:PERRor:FERRor?
Arguments	None
Returns	<freq_error>::=<Nrf> is the frequency error in Hz.
Examples	READ:PERROR:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:PERRor:PEAK? (Query Only)

Returns the peak value in the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
-------------------	--

Group	Read commands
Syntax	READ:PERRor:PEAK?
Related Commands	READ:PERRor:PINdex?
Arguments	None
Returns	<peak>::=<Nrf> is the peak phase error in degrees.
Examples	READ:PERRor:PEAK? might return 0.683, indicating the peak phase error is 0.683 °.

READ:PERRor:PINdex? (Query Only)

Returns the time at the phase error peak.

Conditions	Measurement views: Phase error versus Time
Group	Read commands
Syntax	READ:PERRor:PINdex?
Related Commands	READ:PERRor:PEAK?
Arguments	None
Returns	<peak_time>::=<Nrf> is the time at the phase error peak in symbol number. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	READ:PERRor:PINdex? might return 68.000, indicating that the phase error peak is at symbol #68.

READ:PERRor:RMS (Query Only)

Returns the RMS (Root-Mean-Square) value in the Phase error versus Time measurement.

Conditions Measurement views: Phase error versus Time

Group Read commands

Syntax READ:PERRor:RMS

Arguments None

Returns <rms> ::= <NRf> is the RMS phase error in degrees.

Examples READ:PERRor:RMS might return 0.746, indicating the phase error is 0.746 ° RMS.

READ:PERRor:TRACe? (Query Only)

Returns the Phase error versus Time trace data.

Conditions Measurement views: Phase error versus Time

Group Read commands

Syntax READ:PERRor:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the phase error data for the point n in degrees, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `READ:ERROR:TRACE?` might return `#42036xxxx...` (2036-byte data) for the Phase error versus Time trace.

READ:PHVTime? (Query Only)

Returns the Phase versus Time trace data.

Conditions Measurement views: Phase versus Time

Group Read commands

Syntax `READ:PHVTime?`

Arguments None

Returns `#<num_digit><num_byte><data(1)><data(2)>...<data(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<data(n)>` is the phase in degrees at the n^{th} data point,

4-byte little endian floating-point format specified in IEEE 488.2.

Examples `READ:PHVTIME?` might return `#3160xxxx...` (160-byte data) for the Phase versus Time trace.

READ:PHVTime:MAXimum? (Query Only)

Returns the maximum value in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Read commands

Syntax `READ:PHVTime:MAXimum?`

Related Commands [READ:PHVTime:MAXLocation?](#)

Arguments	None
Returns	<max> ::= <NRf> is the maximum phase in degrees.
Examples	READ:PHVTIME:MAXIMUM? might return 153.8, indicating the maximum phase is 153.8 °.

READ:PHVTime:MAXLocation? (Query Only)

Returns the time at which the phase is maximum.

Conditions	Measurement views: Phase versus Time
Group	Read commands
Syntax	READ:PHVTime:MAXLocation?

Related Commands [READ:PHVTime:MAXimum?](#)

Arguments	None
Returns	<max_time> ::= <NRf> is the time in seconds at which the phase is maximum.
Examples	READ:PHVTIME:MAXLOCATION? might return 175.3E-9, indicating the I or Q level is maximum at 175.3 ns.

READ:PHVTime:MINimum? (Query Only)

Returns the minimum value in the Phase versus Time measurement.

Conditions	Measurement views: Phase versus Time
Group	Read commands
Syntax	READ:PHVTime:MINimum?

Related Commands [READ:PHVTime:MINLocation?](#)

Arguments None

Returns <min>::=<NRF> is the minimum phase in degrees.

Examples READ:PHVTIME:MINIMUM? might return -176.3, indicating the minimum phase is -176.3 °.

READ:PHVTime:MINLocation? (Query Only)

Returns the time at which the phase is minimum.

Conditions Measurement views: Phase versus Time

Group Read commands

Syntax READ:PHVTime:MINLocation?

Related Commands [READ:PHVTime:MINimum?](#)

Arguments None

Returns <min_time>::=<NRF> is the time in seconds at which the phase is minimum.

Examples READ:PHVTIME:MINLOCATION? might return 450.7E-9, indicating the phase is minimum at 450.7 ns.

READ:PHVTime:RESult? (Query Only)

Returns the Phase versus Time measurement results.

Conditions Measurement views: Phase versus Time

Group Read commands

Syntax	READ:PHVTime:RESUlt?
Arguments	None
Returns	<max>, <max_time>, <min>, <min_time> Where <max> ::= <Nrf> is the maximum phase in degrees. <max_time> ::= <Nrf> is the time in seconds at which the phase is maximum. <min> ::= <Nrf> is the minimum phase in degrees. <min_time> ::= <Nrf> is the time in seconds at which the phase is minimum.
Examples	READ:PHVTIME:RESULT? might return 153.8, 175.3E-9, -176.3, 450.7E-9, indicating the maximum phase is 153.8 ° at 175.3 ns and the minimum phase is -176.3 ° at 450.7 ns.

READ:PM:PNEGative? (Query Only)

Returns the negative peak phase deviation (-Pk) in the PM measurement.

Conditions	Measurement views: PM
Group	Read commands
Syntax	READ:PM:PNEGative?
Arguments	None
Returns	<-Pk> ::= <Nrf> is the negative peak phase deviation in degrees.
Examples	READ:PM:PNEGATIVE? might return -23.42, indicating the positive peak phase deviation is -23.42 °.

READ:PM:PPOSitive? (Query Only)

Returns the positive peak phase deviation (+Pk) in the PM measurement.

Conditions	Measurement views: PM
-------------------	-----------------------

Group	Read commands
Syntax	READ:PM:PPOSitive?
Arguments	None
Returns	<+Pk>::=<NRF> is the positive peak phase deviation in degrees.
Examples	READ:PM:PPOSITIVE? might return 26.87, indicating the positive peak phase deviation is 26.87 °.

READ:PM:PTPeak? (Query Only)

Returns the peak-peak phase deviation (Pk-Pk) in the PM measurement.

Conditions	Measurement views: PM
Group	Read commands
Syntax	READ:PM:PTPeak?
Arguments	None
Returns	<Pk-Pk>::=<NRF> is the peak-peak phase deviation in degrees.
Examples	READ:PM:PTPEAK? might return 46.34, indicating the peak-peak phase deviation is 46.34 °.

READ:PM:RESult? (Query Only)

Returns the PM measurement results.

Conditions	Measurement views: PM
Group	Read commands

Syntax	READ:PM:RESu1t?
Arguments	None
Returns	<+Pk> , <-Pk> , <RMS> , <Pk-Pk> Where <+Pk> ::= <NRf> is the positive peak phase deviation in degrees. <-Pk> ::= <NRf> is the negative peak phase deviation in degrees. <RMS> ::= <NRf> is the RMS phase deviation in degrees. <Pk-Pk> ::= <NRf> is the peak-peak phase deviation in degrees.
Examples	READ:PM:RESULT? might return 22.89, -23.45, 15.12, 46.34.

READ:PM:RMS? (Query Only)

Returns the RMS phase deviation in the PM measurement.

Conditions	Measurement views: PM
Group	Read commands
Syntax	READ:PM:RMS?
Arguments	None
Returns	<RMS> ::= <NRf> is the RMS phase deviation in degrees.
Examples	READ:PM:RMS? might return 15.12, indicating the RMS frequency deviation is 15.12 °.

READ:PNOise:ALL? (Query Only)

Returns all results of the phase noise measurement.

Conditions	Measurement views: Phase noise
-------------------	--------------------------------

Group	Read commands
Syntax	READ:PNOise:ALL?
Arguments	None
Returns	<p><Cpower>, <Ferror>, <Pnoise>, <Tjitter>, <Rjitter>, <RFM></p> <p>Where</p> <p><Cpower> ::= <NRf> is the carrier power in dBm. <Ferror> ::= <NRf> is the frequency error in Hz. <Pnoise> ::= <NRf> is the RMS phase noise in degrees. <Tjitter> ::= <NRf> is the total jitter in seconds. <Rjitter> ::= <NRf> is the random jitter in seconds. <RFM> ::= <NRf> is the residual FM in Hz.</p>
Examples	<p>READ:PNOISE:ALL? might return -9.455, 1.235E+6, 51.43, 2.312E-9, 4.178E-9, 14.58, indicating Carrier power: -9.455 dBm, Frequency error: 1.235 MHz, RMS phase noise: 51.43 °, Total jitter: 2.312 ns, Random jitter: 4.178 ns, and Residual FM: 14.58 Hz.</p>

READ:PNOise:CARRier:FERRor? (Query Only)

Returns the carrier frequency error in the phase noise measurement.

Conditions	Measurement views: Phase noise
Group	Read commands
Syntax	READ:PNOise:CARRier:FERRor?
Arguments	None
Returns	<NRf> Carrier frequency error in Hz.

Examples `READ:PNOISE:CARRIER:FERROR?` might return `1.235E+6`, indicating that the carrier frequency error is 1.235 MHz.

READ:PNOise:CARRier:POWer? (Query Only)

Returns the carrier power in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Read commands

Syntax `READ:PNOise:CARRier:POWer?`

Arguments None

Returns `<NRf>` Carrier power in dBm.
The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `READ:PNOISE:CARRIER:POWER?` might return `-9.455`, indicating that the carrier power is -9.455 dBm.

READ:PNOise:JITTer? (Query Only)

Returns the jitter in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Read commands

Syntax `READ:PNOise:JITTer?`

Arguments None

Returns `<NRf>` Jitter in seconds.

Examples `READ:PNOISE:JITTER?` might return `2.312E-9`, indicating that the jitter is 2.312 ns.

READ:PNOise:RESidual:FM? (Query Only)

Returns the residual FM in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Read commands

Syntax `READ:PNOise:RESidual:FM?`

Arguments None

Returns <NRf> Residual FM in Hz.

Examples `READ:PNOISE:RESIDUAL:FM?` might return `14.58`, indicating that the residual FM is 14.58 Hz.

READ:PNOise:RMS:PNOise? (Query Only)

Returns the RMS phase noise in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Read commands

Syntax `READ:PNOise:RMS:PNOise?`

Arguments None

Returns <NRf> RMS phase noise in degrees.

Examples `READ:PNOISE:RMS:PNOISE?` might return `51.43`, indicating that the RMS phase noise is 51.43 °.

READ:PNOise:SPECtrum<x>:X? (Query Only)

Returns the frequencies of the specified trace.

The parameter <x> = 1 and 2, representing Trace 1 and Trace 2, respectively.

Conditions Measurement views: Phase noise

Group Read commands

Syntax READ:PNOise:SPECtrum<x>:X?

Arguments None

Returns #<num_digit><num_byte><x(1)><x(2)>...<x(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<x(n)> is the frequency (Hz) at the nth point,

4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:PNOISE:SPECTRUM1:X? might return #516020xxxx... (16020-byte data) for the frequencies of Trace 1.

READ:PNOise:SPECtrum<x>:XY? (Query Only)

Returns the frequency and phase noise pairs of the specified trace.

The parameter <x> = 1 and 2, representing Trace 1 and Trace 2, respectively.

Conditions Measurement views: Phase noise

Group Read commands

Syntax READ:PNOise:SPECtrum<x>:XY?

Arguments None

Returns #<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)> . . . <x(n)><y(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<x(n)><y(n)> is the frequency (Hz) and phase noise (dBc/Hz) pair at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:PNOISE:SPECTRUM1:XY? might return #516020xxxx . . . (16020-byte data) for the frequency and phase noise pairs of the Trace 1.

READ:PNOise:SPECTrum<x>[:Y]? (Query Only)

Returns the phase noise values of the specified trace.

The parameter <x> = 1 and 2, representing Trace 1 and Trace 2, respectively.

Conditions Measurement views: Phase noise

Group Read commands

Syntax READ:PNOise:SPECTrum<x>[:Y]?

Arguments None

Returns #<num_digit><num_byte><y(1)><y(2)> . . . <y(n)>

Where <num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<y(n)> is the phase noise (dBc/Hz) at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:PNOISE:SPECTRUM1:Y might return #516020xxxx . . . (16020-byte data) for the phase noise values of Trace 1.

READ:PULSe[:RESult]:ATX? (Query Only)

Returns the average transmitted power in the pulse table.

Conditions Measurement views: Pulse table

Group	Read commands
Syntax	READ:PULSE[:RESuLt]:ATX?
Arguments	None
Returns	<p><first_pulse_num>, <ATX(1)>, < ATX(2)>, ... <ATX(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <ATX(n)> ::= <NRf> is the average transmitted power for the pulse with the number of [first_pulse_num + n - 1] in dBm. The unit can be changed to watts by the [SENSE]:POWER:UNITs command. Volt is invalid in the average transmitted power measurement.</p>
Examples	READ:PULSE:RESULT:ATX? might return 0, -18.57, -18.73, -18.20, -18.53 for Pulse 0 to 3.

READ:PULSE[:RESuLt]:AVERAge? (Query Only)

Returns the average on power in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSE[:RESuLt]:AVERAge?
Arguments	None
Returns	<p><first_pulse_num>, <avg(1)>, < avg(2)>, ... <avg(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <avg(n)> ::= <NRf> is the average on power for the pulse with the number of [first_pulse_num + n - 1] in dBm. The unit can be changed by the [SENSE]:POWER:UNITs command.</p>

Examples READ:PULSE:RESULT:AVERAGE? might return
0, -2.354, -2.368, -2.343, -2.358 for Pulse 0 to 3.

READ:PULSe[:RESuLt]:DRoDb? (Query Only)

Returns the droop in dB in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESuLt]:DRoDb?

Related Commands [READ:PULSe\[:RESuLt\]:DRoOp?](#)

Arguments None

Returns <first_pulse_num>, <droop(1)>, <droop(2)>, ... <droop(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<droop(n)>::=<NRf> is the wattage droop for the pulse with the number of
[first_pulse_num + n - 1] in dB.

Examples READ:PULSE:RESULT:DRoDb? might return 1, -0.4, 0.32, 0.2, -0.1 for
Pulse 1 to 4.

READ:PULSe[:RESuLt]:DRoOp? (Query Only)

Returns the average on power in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESuLt]:DRoOp?

Related Commands [READ:PULSe\[:RESult\]:DRODb?](#)

Arguments None

Returns <first_pulse_num>, <droop(1)>, <droop(2)>, ... <droop(n)>

Where

<first_pulse_num> ::= <NR1> is the first pulse number.

<droop(n)> ::= <NRf> is the wattage droop for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Examples READ:PULSE:RESULT:DROOP? might return 0, -270.9E-3, -193.0E-3, -242.7E-3, -177.5E-3 for Pulse 0 to 3.

READ:PULSe[:RESult]:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESult]:DUTPct?

Arguments None

Returns <first_pulse_num>, <duty_pct(1)>, <duty_pct(2)>, ... <duty_pct(n)>

Where

<first_pulse_num> ::= <NR1> is the first pulse number.

<duty_pct(n)> ::= <NRf> is the duty factor for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Examples READ:PULSE:RESULT:DUTPCT? might return 0, 28.94, 28.96, 29.00, 29.01 for Pulse 0 to 3.

READ:PULSe[:RESuLt]:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSe[:RESuLt]:DUTRatio?
Arguments	None
Returns	<p><first_pulse_num>, <duty_ratio(1)>, <duty_ratio(2)>, ... <duty_ratio(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <duty_ratio(n)> ::= <NRf> is the duty factor for the pulse with the number of [first_pulse_num + n - 1] (no unit).</p>
Examples	READ:PULSE:RESULT:DUTRATIO? might return 0, 289.4E-3, 289.6E-3, 290.0E-3, 290.1E-3 for Pulse 0 to 3.

READ:PULSe[:RESuLt]:FALL? (Query Only)

Returns the fall time in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSe[:RESuLt]:FALL?
Arguments	None
Returns	<p><first_pulse_num>, <fall(1)>, <fall(2)>, ... <fall(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number.</p>

`<fall(n)> ::= <NRf>` is the fall time for the pulse with the number of `[first_pulse_num + n - 1]` in seconds.

Examples `READ:PULSE:RESULT:FALL?` might return `0,110.3E-9,90.45E-9,95.03E-9,111.9E-9` for Pulse 0 to 3.

READ:PULSe[:RESult]:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax `READ:PULSe[:RESult]:FRDeviation?`

Arguments None

Returns `<first_pulse_num>,<freq_dev(1)>,<freq_dev(2)>,...<freq_dev(n)>`

Where

`<first_pulse_num> ::= <NR1>` is the first pulse number.

`<freq_dev(n)> ::= <NRf>` is the frequency deviation for the pulse with the number of `[first_pulse_num + n - 1]` in Hz.

Examples `READ:PULSE:RESULT:FRDEVIATION?` might return `1,740.6E+3,736.5E+3,718.3E+3,672.2E+3` for Pulse 1 to 4.

READ:PULSe[:RESult]:IRAMplitude? (Query Only)

Returns the pulse impulse response amplitude in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax `READ:PULSe[:RESult]:IRAMplitude?`

Returns <first_pulse_num>, <amplitude(1)>, <amplitude(2)>, ... <amplitude(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<amplitude(n)>::=<NRf> is the sidelobe level, in dB, from the mainlobe for the pulse with the number of [first_pulse_num + n - 1].

Examples READ:PULSE[:RESULT]:IRAMPLITUDE? might return
1.0000000000, -45.3, -47.5, -50.2 for Pulse 1 through 3.

READ:PULSE[:RESULT]:IRTime? (Query Only)

Returns the impulse response time in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSE[:RESULT]:IRTime?

Returns <first_pulse_num>, <time(1)>, <time(2)>, ... <time(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<time(n)>::=<NRf> is the sidelobe offset time from the mainlobe for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Examples READ:PULSE[:RESULT]:IRTIME? might return
1.0000000000, 806.6708687693E-9, -846.6595318168E-9, -873.3477443457E-9
for Pulse 1 to 3.

READ:PULSE[:RESULT]:MFReqerror? (Query Only)

Returns the maximum frequency error in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax	READ:PULSE[:RESuLt]:MFreqerror?
Arguments	None
Returns	<first_pulse_num>, <max_freq_err(1)>, <max_freq_err(2)>, ... <max_freq_err(n)>
	Where <first_pulse_num>::=<NR1> is the first pulse number. <max_freq_err(n)>::=<NRf> is the maximum frequency error for the pulse with the number of [first_pulse_num + n - 1] in Hz.
Examples	READ:PULSE:RESULT:MFREQERROR? might return 1, 597.5E+3, 675.8E+3, 642.8E+3, 598.2E+3 for Pulse 1 to 4.

READ:PULSE[:RESuLt]:MPHerror? (Query Only)

Returns the maximum phase error in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSE[:RESuLt]:MPHerror?
Arguments	None
Returns	<first_pulse_num>, <max_phase_err(1)>, <max_phase_err(2)>, ... <max_phase_err(n)>
	Where <first_pulse_num>::=<NR1> is the first pulse number. <max_phase_err(n)>::=<NRf> is the maximum phase error for the pulse with the number of [first_pulse_num + n - 1] in degrees.
Examples	READ:PULSE:RESULT:MPHERROR? might return 1, -9.221, -8.413, -11.853, -10.258 for Pulse 1 to 4.

READ:PULSe[:RESuLt]:OVEDb? (Query Only)

Returns the overshoot in dB in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSe[:RESuLt]:OVEDb?
Related Commands	READ:PULSe[:RESuLt]:OVERshoot?
Arguments	None
Returns	<code><first_pulse_num></code> , <code><overshoot(1)></code> , <code><overshoot(2)></code> , ... <code><overshoot(n)></code> Where <code><first_pulse_num> ::= <NR1></code> is the first pulse number. <code><overshoot(n)> ::= <NRf></code> is the overshoot for the pulse with the number of [<code>first_pulse_num + n - 1</code>] in dB.
Examples	READ:PULSE:RESULT:OVERDB? might return 1, 1.2, 2.3, 1.0, 0.2 for Pulse 1 to 4.

READ:PULSe[:RESuLt]:OVERshoot? (Query Only)

Returns the overshoot in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSe[:RESuLt]:OVERshoot?
Related Commands	READ:PULSe[:RESuLt]:OVEDb?
Arguments	None

Returns <first_pulse_num>, <overshoot(1)>, <overshoot(2)>, ... <overshoot(n)>

Where

<first_pulse_num> ::= <NR1> is the first pulse number.

<overshoot(n)> ::= <NRf> is the overshoot for the pulse with the number of [first_pulse_num + n - 1] in percent (%) of watts or volts.

Examples READ:PULSE:RESULT:OVERSHOOT? might return 1, 1.2, 2.3, 1.0, 0.2 for Pulse 1 through 4.

READ:PULSe[:RESult]:PHDeviation? (Query Only)

Returns the phase deviation in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESult]:PHDeviation?

Arguments None

Returns <first_pulse_num>, <phase_dev(1)>, <phase_dev(2)>, ...
<phase_dev(n)>

Where

<first_pulse_num> ::= <NR1> is the first pulse number.

<phase_dev(n)> ::= <NRf> is the phase deviation for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Examples READ:PULSE:RESULT:PHDEVIATION? might return 1, 11.658, 9.640, 10.509, 8.272 for Pulse 1 to 4.

READ:PULSe[:RESult]:PPFRequency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse table.

Conditions Measurement views: Pulse table

Group	Read commands
Syntax	READ:PULSE[:RESuLt]:PPFrequency?
Arguments	None
Returns	<p><first_pulse_num>, <pp_freq(1)>, <pp_freq(2)>, . . . <pp_freq(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <pp_freq(n)> ::= <NRf> is the pulse-pulse carrier frequency for the pulse with the number of [first_pulse_num + n - 1] in Hz.</p>
Examples	<p>READ:PULSE:RESULT:PPFREQUENCY? might return 0, 0.000, 1.258E+3, -3.121E+3, 1.862E+3 for Pulse 0 to 3.</p>

READ:PULSE[:RESuLt]:PPOWer? (Query Only)

Returns the peak power in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSE[:RESuLt]:PPOWer?
Arguments	None
Returns	<p><first_pulse_num>, <pk_power(1)>, <pk_power(2)>, . . . <pk_power(n)></p> <p>Where <first_pulse_num> ::= <NR1> is the first pulse number. <pk_power(n)> ::= <NRf> is the peak power for the pulse with the number of [first_pulse_num + n - 1] in dBm. The unit can be changed by the [SENSE]:POWER:UNITs command.</p>

Examples READ:PULSE:RESULT:PPOWER? might return 0, -2.26, -2.27, -2.23, -2.25 for Pulse 0 to 3.

READ:PULSe[:RESult]:PPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESult]:PPHase?

Arguments None

Returns <first_pulse_num>, <pp_phase(1)>, <pp_phase(2)>, . . . <pp_phase(n)>

Where

<first_pulse_num> ::= <NR1> is the first pulse number.

<pp_phase(n)> ::= <NRf> is the pulse-pulse carrier phase for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Examples READ:PULSE:RESULT:PPHASE? might return 0, 0.000, 21.66, 46.76, 57.56 for Pulse 0 to 3.

READ:PULSe[:RESult]:RINTerval? (Query Only)

Returns the repetition interval in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESult]:RINTerval?

Arguments None

Returns <first_pulse_num>, <rep_int(1)>, <rep_int(2)>, ... <rep_int(n)>
 Where
 <first_pulse_num>::=<NR1> is the first pulse number.
 <rep_int(n)>::=<NRf> is the repetition interval for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Examples READ:PULSE:RESULT:RINTERVAL? might return 0, 16.03E-6, 16.08E-6, 16.07E-6, 16.02E-6 for Pulse 0 to 3.

READ:PULSe[:RESuLt]:RIPDb? (Query Only)

Returns the ripple in dB in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESuLt]:RIPDb?

Related Commands [READ:PULSe\[:RESuLt\]:RIPPlE?](#)

Arguments None

Returns <first_pulse_num>, <ripple(1)>, <ripple(2)>, ... <ripple(n)>
 Where
 <first_pulse_num>::=<NR1> is the first pulse number.
 <ripple(n)>::=<NRf> is the ripple for the pulse with the number of [first_pulse_num + n - 1] in dB.

Examples READ:PULSE:RESULT:RIPDB? might return 1, 0.4, 0.32, 0.2, 0.1 for Pulse 1 to 4.

READ:PULSe[:RESuLt]:RIPPlE? (Query Only)

Returns the ripple in the pulse table.

Conditions Measurement views: Pulse table

Group	Read commands
Syntax	READ:PULSE[:RESult]:RIPPlE?
Related Commands	READ:PULSE[:RESult]:RIPDb?
Arguments	None
Returns	<first_pulse_num>,<ripple(1)>,<ripple(2)>,...<ripple(n)> Where <first_pulse_num>::=<NR1> is the first pulse number. <ripple(n)>::=<NRf> is the watt or voltage ripple for the pulse with the number of [first_pulse_num + n - 1] in percent (%).
Examples	READ:PULSE:RESULT:RIPPLE? might return 0,106.5E-3,177.6E-3,148.3E-3,148.5E-3 for Pulse 0 to 3.

READ:PULSE[:RESult]:RISE? (Query Only)

Returns the rise time in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSE[:RESult]:RISE?
Arguments	None
Returns	<first_pulse_num>,<rise(1)>,<rise(2)>,...<rise(n)> Where <first_pulse_num>::=<NR1> is the first pulse number. <rise(n)>::=<NRf> is the rise time for the pulse with the number of [first_pulse_num + n - 1] in seconds.
Examples	READ:PULSE:RESULT:RISE? might return 0,92.94E-9,115.9E-9,115.1E-9,97.45E-9 for Pulse 0 to 3.

READ:PULSe[:RESuLt]:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESuLt]:RMSFreqerror?

Arguments None

Returns <first_pulse_num>, <RMS_freq_err(1)>, <RMS_freq_err(2)>, ...
<RMS_freq_err(n)>

Where

<first_pulse_num> ::= <NR1> is the first pulse number.

<RMS_freq_err(n)> ::= <NRf> is the RMS frequency error for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Examples READ:PULSE:RESULT:RMSFREQERROR? might return 1, 51.54E+3, 69.20E+3, 64.21E+3, 51.02E+3 for Pulse 1 to 4.

READ:PULSe[:RESuLt]:RMSPherror? (Query Only)

Returns the RMS phase error in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax READ:PULSe[:RESuLt]:RMSPherror?

Arguments None

Returns <first_pulse_num>, <RMS_phase_err(1)>, <RMS_phase_err(2)>, ...
<RMS_phase_err(n)>

Where

`<first_pulse_num>::=<NR1>` is the first pulse number.
`<RMS_phase_err(n)>::=<NRf>` is the RMS phase error for the pulse with the number of `[first_pulse_num + n - 1]` in degrees.

Examples `READ:PULSE:RESULT:RMSPHERROR?` might return
`1,908.4E-3,752.8E-3,981.7E-3,886.4E-3` for Pulse 1 to 4.

READ:PULSe[:RESUlt]:RRATe? (Query Only)

Returns the repetition rate in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax `READ:PULSe[:RESUlt]:RRATe?`

Arguments None

Returns `<first_pulse_num>, <rep_rate(1)>, <rep_rate(2)>, ...`
`<rep_rate(n)>`

Where

`<first_pulse_num>::=<NR1>` is the first pulse number.

`<rep_rate(n)>::=<NRf>` is the repetition rate for the pulse with the number of `[first_pulse_num + n - 1]` in Hz.

Examples `READ:PULSE:RESULT:RRATE?` might return `0,62.50E+3,62.52E+3,`
`62.51E+3,62.49E+3` for Pulse 0 to 3.

READ:PULSe[:RESUlt]:TIME? (Query Only)

Returns the time in the pulse table.

Conditions Measurement views: Pulse table

Group Read commands

Syntax	READ:PULSE[:RESuLt]:TIME?
Arguments	None
Returns	<first_pulse_num>, <time(1)>, <time(2)>, ... <time(n)> Where <first_pulse_num> ::= <NR1> is the first pulse number. <time(n)> ::= <NRf> is the time for the pulse with the number of [first_pulse_num + n - 1] in seconds.
Examples	READ:PULSE:RESULT:TIME? might return 1, 7.937E-3, 8.436E-3, 6.504E-3, 9.876E-3 for Pulse 1 to 4.

READ:PULSE[:RESuLt]:WIDTh? (Query Only)

Returns the pulse width in the pulse table.

Conditions	Measurement views: Pulse table
Group	Read commands
Syntax	READ:PULSE[:RESuLt]:WIDTh?
Arguments	None
Returns	<first_pulse_num>, <width(1)>, <width(2)>, ... <width(n)> Where <first_pulse_num> ::= <NR1> is the first pulse number. <width(n)> ::= <NRf> is the pulse width for the pulse with the number of [first_pulse_num + n - 1] in seconds.
Examples	READ:PULSE:RESULT:WIDTh? might return 0, 4.630E-6, 4.632E-6, 4.639E-6, 4.642E-6 for Pulse 0 to 3.

READ:PULSE:STATistics? (Query Only)

Returns the trace data of the pulse statistics measurement selected by the [DISPlay:PULSE:SElect:RESuLt](#) command.

NOTE. Select the plot type (Trend, FFT, Time Trend or Histogram) using the `DISPlay:PULSe:STATistics:PLOT` command before executing this query.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	<code>READ:PULSe:STATistics?</code>
Arguments	None
Returns	<p><code>#<num_digit><num_byte><data(1)><data(2)>...<data(n)></code></p> <p>Where</p> <ul style="list-style-type: none"> <code><num_digit></code> is the number of digits in <code><num_byte></code>. <code><num_byte></code> is the number of bytes of data that follow. <code><data(n)></code> is the amplitude at the n^{th} data point. <p>The unit is current measurement unit (Plot = Trend or Time Trend), dB (Plot = FFT), count or percent (Plot = Histogram)</p> <p>4-byte little endian floating-point format specified in IEEE 488.2.</p> <p>The unit of power is selected by the <code>[SENSe]:POWER:UNITs</code> command.</p>
Examples	<p><code>READ:PULSE:STATISTICS?</code> might return <code>#264xxxx...</code> (64-byte data) for the statistics trace of the pulse width measurement when <code>DISPlay:PULSe:SElect:RESult</code> is set to <code>WIDTh</code>.</p>

READ:PULSe:STATistics:ATX? (Query Only)

Returns the average transmitted power in the pulse statistics. This command is valid when `DISPlay:PULSe:STATistics:PLOT` is set to `TREND`.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	<code>READ:PULSe:STATistics:ATX?</code>
Arguments	None

Returns <ATX_avg>, <ATX_min>, <ATX_max>

Where

<ATX_avg> ::= <NRf> is the average of the average transmitted power.

<ATX_min> ::= <NRf> is the minimum of the average transmitted power.

<ATX_max> ::= <NRf> is the maximum of the average transmitted power.

Unit: dBm.

The unit can be changed to watts by the [\[SENSe\]:POWer:UNITs](#) command.

Volt is invalid in the average transmitted power measurement.

Examples READ:PULSE:STATISTICS:ATX? might return -18.51, -18.74, -18.12 for the average transmitted power in the pulse statistics.

READ:PULSe:STATistics:AVERage? (Query Only)

Returns the average on power in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:AVERage?

Arguments None

Returns <avg_avg>, <avg_min>, < avg_max>

Where

<avg_avg> ::= <NRf> is the average of the average on power.

<avg_min> ::= <NRf> is the minimum of the average on power.

<avg_max> ::= <NRf> is the maximum of the average on power.

Unit: dBm.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples READ:PULSE:STATISTICS:AVERAGE? might return -2.35, -2.36, -2.34 for the average on power in the pulse statistics.

READ:PULSe:STATistics:DRoDb? (Query Only)

Returns the droop in dB in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:DRoDb?

Related Commands [READ:PULSe:STATistics:DRoOp?](#)

Arguments None

Returns <droop_avg>, <droop_min>, <droop_max>

Where

<droop_avg> ::= <NRf> is the average droop.

<droop_min> ::= <NRf> is the minimum droop.

<droop_max> ::= <NRf> is the maximum droop.

Unit: in dB by watts.

Examples READ:PULSE:STATISTICS:DRoDb? might return 22.67E-3, -613.5E-3, 633.8E-3 for the droop in the pulse statistics.

READ:PULSe:STATistics:DRoOp? (Query Only)

Returns the droop in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:DRoOp?

Related Commands [READ:PULSe:STATistics:DRoDb?](#)

Arguments None

Returns <droop_avg>, <droop_min>, <droop_max>

Where

<droop_avg> ::= <NRf> is the average droop.

<droop_min> ::= <NRf> is the minimum droop.

<droop_max> ::= <NRf> is the maximum droop.

Unit: Percent (%) by watts.

Examples READ:PULSE:STATISTICS:DROOP? might return 22.67E-3, -613.5E-3, 633.8E-3 for the droop in the pulse statistics.

READ:PULSe:STATistics:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TRENd.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:DUTPct?

Related Commands

Arguments None

Returns <duty_pct_avg>, <duty_pct_min>, <duty_pct_max>

Where

<duty_pct_avg> ::= <NRf> is the average duty factor.

<duty_pct_min> ::= <NRf> is the minimum duty factor.

<duty_pct_max> ::= <NRf> is the maximum duty factor.

Unit: Percent (%).

Examples READ:PULSE:STATISTICS:DUTPCT? might return 2.437, 2.310, 2.657 for the duty factor (%) in the pulse statistics.

READ:PULSe:STATistics:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:DUTRatio?
Arguments	None
Returns	<code><duty_ratio_avg>, <duty_ratio_min>, <duty_ratio_max></code> Where <code><duty_ratio_avg>::=<NRf></code> is the average duty factor. <code><duty_ratio_min>::=<NRf></code> is the minimum duty factor. <code><duty_ratio_max>::=<NRf></code> is the maximum duty factor. Unit: None.
Examples	READ:PULSE:STATISTICS:DUTRATIO? might return 24.37E-3, 23.11E-3, 26.57E-3 for the duty factor (ratio) in the pulse statistics.

READ:PULSe:STATistics:FALL? (Query Only)

Returns the fall time in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:FALL?
Arguments	None
Returns	<code><fall_avg>, <fall_min>, <fall_max></code>

Where
 <fall_avg>::=<NRf> is the average fall time.
 <fall_min>::=<NRf> is the minimum fall time.
 <fall_max>::=<NRf> is the maximum fall time.
 Unit: Seconds.

Examples READ:PULSE:STATISTICS:FALL? might return 70.27E-9, 69.62E-9, 71.27E-9 for the fall time in the pulse statistics.

READ:PULSe:STATistics:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:FRDeviation?

Arguments None

Returns <freq_dev_avg>, <freq_dev_min>, <freq_dev_max>

Where
 <freq_dev_avg>::=<NRf> is the average frequency deviation.
 <freq_dev_min>::=<NRf> is the minimum frequency deviation.
 <freq_dev_max>::=<NRf> is the maximum frequency deviation.
 Unit: Hz.

Examples READ:PULSE:STATISTICS:FRDEVIATION? might return 754.1E+3, 660.5E+3, 835.2E+3 for the frequency deviation in the pulse statistics.

READ:PULSe:STATistics:IRAMplitude? (Query Only)

Returns the Pulse Impulse Response amplitude measurement in the pulse statistics.

Conditions Measurement views: Pulse statistics

Group	Read commands
Syntax	READ:PULSE:STATISTICS:IRAmplitude?
Returns	<p><amp_avg>, <amp_min>, <amp_max></p> <p>Where</p> <p><amp_avg> ::= <NRF> is the average of the impulse response amplitude.</p> <p><amp_min> ::= <NRF> is the minimum of the impulse response amplitude.</p> <p><amp_max> ::= <NRF> is the maximum of impulse response amplitude.</p> <p>Unit: dB.</p>
Examples	READ:PULSE:STATISTICS:IRAMPLITUDE? might return -45.3, -47.1, -43.2 for the impulse response amplitude in the pulse statistics.

READ:PULSE:STATISTICS:IRTime? (Query Only)

Returns the impulse response time in the pulse statistics.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSE:STATISTICS:IRTime?
Returns	<p><avg_avg>, <avg_min>, <avg_max></p> <p>Where</p> <p><avg_avg> ::= <NRF> is the average of the impulse response time.</p> <p><avg_min> ::= <NRF> is the minimum of the impulse response time.</p> <p><avg_max> ::= <NRF> is the maximum of impulse response time.</p> <p>Unit: seconds.</p>
Examples	READ:PULSE:STATISTICS:IRTIME? might return -2.35, -2.36, -2.34 for the impulse response time in the pulse statistics.

READ:PULSe:STATistics:MFReqerror? (Query Only)

Returns the maximum frequency error in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:MFReqerror?

Arguments None

Returns <max_freq_err_avg>, <max_freq_err_min>, <max_freq_err_max>

Where

<max_freq_err_avg>::=<NRf> is the average of maximum frequency error.

<max_freq_err_min>::=<NRf> is the minimum of maximum frequency error.

<max_freq_err_max>::=<NRf> is the maximum of maximum frequency error.

Unit: Hz.

Examples READ:PULSE:STATISTICS:MFREQERROR? might return
645.0E+3, 555.6E+3, 738.8E+3 for the maximum frequency error
in the pulse statistics.

READ:PULSe:STATistics:MPHerror? (Query Only)

Returns the maximum phase error in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:MPHerror?

Arguments None

Returns <max_phase_err_avg>, <max_phase_err_min>, <max_phase_err_max>

Where

<max_phase_err_avg> ::= <NRf> is the average of maximum phase error.

<max_phase_err_min> ::= <NRf> is the minimum of maximum phase error.

<max_phase_err_max> ::= <NRf> is the maximum of maximum phase error.

Unit: Degrees.

Examples READ:PULSE:STATISTICS:MPHERROR? might return -11.47, -17.18, -7.61 for the maximum phase error in the pulse statistics.

READ:PULSe:STATistics:OVEDb? (Query Only)

Returns the overshoot measurement result in dB in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND or TTRend.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:OVEDb?

Related Commands [READ:PULSe:STATistics:OVERshoot?](#)

Arguments None

Returns <overshoot_avg>, <overshoot_min>, <overshoot_max>

Where

<overshoot_avg> ::= <NRf> is the average overshoot.

<overshoot_min> ::= <NRf> is the minimum overshoot.

<overshoot_max> ::= <NRf> is the maximum overshoot.

Unit: dB.

Examples READ:PULSE:STATISTICS:OVEDB? might return 0.3, 0.1, 0.5 for the overshoot measurement result in dB in the pulse statistics.

READ:PULSe:STATistics:OVERshoot? (Query Only)

Returns the overshoot in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TRENd or TTRend.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:OVERshoot?
Related Commands	READ:PULSe:STATistics:OVEDb?
Arguments	None
Returns	<overshoot_avg>, <overshoot_min>, <overshoot_max> Where <overshoot_avg> ::= <NRf> is the average overshoot. <overshoot_min> ::= <NRf> is the minimum overshoot. <overshoot_max> ::= <NRf> is the maximum overshoot. Unit: Percent (%) as watts or volts.
Examples	READ:PULSE:STATISTICS:OVERSHOOT? might return 0.3, 0.1, 0.5 for the overshoot in the pulse statistics.

READ:PULSe:STATistics:PHDeviation? (Query Only)

Returns the phase deviation in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TRENd.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:PHDeviation?
Arguments	None

Returns <phase_dev_avg>, <phase_dev_min>, <phase_dev_max>

Where

<phase_dev_avg> ::= <NRf> is the average phase deviation.

<phase_dev_min> ::= <NRf> is the minimum phase deviation.

<phase_dev_max> ::= <NRf> is the maximum phase deviation.

Unit: Degrees.

Examples READ:PULSE:STATISTICS:PHDEVIATION? might return 11.678, 7.694, 17.374 for the phase deviation in the pulse statistics.

READ:PULSe:STATistics:PPFrequency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:PPFrequency?

Arguments None

Returns <pp_freq_avg>, <pp_freq_min> >, <pp_freq_max>

Where

<pp_freq_avg> ::= <NRf> is the average pulse-pulse carrier frequency.

<pp_freq_min> ::= <NRf> is the minimum pulse-pulse carrier frequency.

<pp_freq_max> ::= <NRf> is the maximum pulse-pulse carrier frequency.

Unit: Hz.

Examples READ:PULSE:STATISTICS:PPFREQUENCY? might return 1.135E+3, 311.3E+3, -262.8E+3 for the pulse-pulse carrier frequency in the pulse statistics.

READ:PULSe:STATistics:PPOWer? (Query Only)

Returns the peak power in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSE:STATistics:PPOWER?
Arguments	None
Returns	<p><pk_power_avg>, <pk_power_min>, <pk_power_max></p> <p>Where</p> <p><pk_power_avg> ::= <NRf> is the average peak power.</p> <p><pk_power_min> ::= <NRf> is the minimum peak power.</p> <p><pk_power_max> ::= <NRf> is the maximum peak power.</p> <p>Unit: dBm.</p> <p>The unit can be changed by the [SENSE]:POWER:UNITs command.</p>
Examples	READ:PULSE:STATistics:PPOWER? might return -2.273, -2.313, -2.235 for the peak power in the pulse statistics.

READ:PULSE:STATistics:PPPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse statistics. This command is valid when [DISPlay:PULSE:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSE:STATistics:PPPHase?
Arguments	None
Returns	<p><pp_phase_avg>, <pp_phase_min>, <pp_phase_max></p> <p>Where</p> <p><pp_phase_avg> ::= <NRf> is the average pulse-pulse carrier phase.</p> <p><pp_phase_min> ::= <NRf> is the minimum pulse-pulse carrier phase.</p> <p><pp_phase_max> ::= <NRf> is the maximum pulse-pulse carrier phase.</p>

Unit: Degrees.

Examples `READ:PULSE:STATISTICS:PPPHASE?` might return `-9.298E-3,-254.3E-3,311.7E-3` for the pulse-pulse carrier phase in the pulse statistics.

READ:PULSe:STATistics:RINteRval? (Query Only)

Returns the repetition interval in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax `READ:PULSe:STATistics:RINteRval?`

Arguments None

Returns `<rep_int_avg>,<rep_int_min>,<rep_int_max>`

Where

`<rep_int_avg>::=<NRf>` is the average repetition interval.

`<rep_int_min>::=<NRf>` is the minimum repetition interval.

`<rep_int_max>::=<NRf>` is the maximum repetition interval.

Unit: Seconds.

Examples `READ:PULSE:STATISTICS:RINTERVAL?` might return `240.5E-6,217.9E-6,281.2E-6` for the repetition interval in the pulse statistics.

READ:PULSe:STATistics:RIPDb? (Query Only)

Returns the ripple in dB in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSE:STATISTICS:RIPDb?

Related Commands [READ:PULSE:STATISTICS:RIPPLE?](#)

Arguments None

Returns <ripple_avg>, <ripple_min>, <ripple_max>

Where

<ripple_avg>::=<NRf> is the average ripple.

<ripple_min>::=<NRf> is the minimum ripple.

<ripple_max>::=<NRf> is the maximum ripple.

Unit: dB.

Examples READ:PULSE:STATISTICS:RIPDB? might return
160.4E-3, 83.78E-3, 287.7E-3 for the ripple in dB in the pulse statistics.

READ:PULSE:STATISTICS:RIPPLE? (Query Only)

Returns the ripple in the pulse statistics. This command is valid when [DISPLAY:PULSE:STATISTICS:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSE:STATISTICS:RIPPLE?

Related Commands [READ:PULSE:STATISTICS:RIPDb?](#)

Arguments None

Returns <ripple_avg>, <ripple_min>, <ripple_max>

Where

<ripple_avg>::=<NRf> is the average ripple.

<ripple_min>::=<NRf> is the minimum ripple.

<ripple_max>::=<NRf> is the maximum ripple.

Unit: Percent (%) as watts or volts.

Examples READ:PULSE:STATISTICS:RIPPLE? might return 160.4E-3, 83.78E-3, 287.7E-3 for the ripple in the pulse statistics.

READ:PULSe:STATistics:RISE? (Query Only)

Returns the rise time in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:RISE?

Arguments None

Returns <rise_avg>, <rise_min>, <rise_max>

Where

<rise_avg>::=<NRf> is the average rise time.

<rise_min>::=<NRf> is the minimum rise time.

<rise_max>::=<NRf> is the maximum rise time.

Unit: Seconds.

Examples READ:PULSE:STATISTICS:RISE? might return 105.4E-9, 91.65E-9, 116.2E-9 for the rise time in the pulse statistics.

READ:PULSe:STATistics:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax READ:PULSe:STATistics:RMSFreqerror?

Arguments	None
Returns	<p><RMS_freq_err_avg>, <RMS_freq_err_min>, <RMS_freq_err_max></p> <p>Where</p> <p><RMS_freq_err_avg> ::= <NRf> is the average of RMS frequency error.</p> <p><RMS_freq_err_min> ::= <NRf> is the minimum of RMS frequency error.</p> <p><RMS_freq_err_max> ::= <NRf> is the maximum of RMS frequency error.</p> <p>Unit: Hz.</p>
Examples	<p>READ:PULSE:STATISTICS:RMSFREQERROR? might return 63.67E+3, 45.49E+3, 81.28E+3 for the RMS frequency error in the pulse statistics.</p>

READ:PULSe:STATistics:RMSPherror? (Query Only)

Returns the RMS phase error in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TRENd.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:RMSPherror?
Arguments	None
Returns	<p><RMS_phase_err_avg>, <RMS_phase_err_min>, <RMS_phase_err_max></p> <p>Where</p> <p><RMS_phase_err_avg> ::= <NRf> is the average of RMS phase error.</p> <p><RMS_phase_err_min> ::= <NRf> is the minimum of RMS phase error.</p> <p><RMS_phase_err_max> ::= <NRf> is the maximum of RMS phase error.</p> <p>Unit: Degrees.</p>
Examples	<p>READ:PULSE:STATISTICS:RMSPHERROR? might return 1.032, 604.5E-3, 1.606 for the RMS phase error in the pulse statistics.</p>

READ:PULSe:STATistics:RRATe? (Query Only)

Returns the repetition rate in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:RRATe?
Arguments	None
Returns	<code><rep_rate_avg></code> , <code><rep_rate_min></code> , <code><rep_rate_max></code> Where <code><rep_rate_avg> ::= <NRf></code> is the average repetition rate. <code><rep_rate_min> ::= <NRf></code> is the minimum repetition rate. <code><rep_rate_max> ::= <NRf></code> is the maximum repetition rate. Unit: Hz.
Examples	READ:PULSE:STATISTICS:RRATE? might return 62.50E+3, 62.49E+3, 62.52E+3 for the repetition rate in the pulse statistics.

READ:PULSe:STATistics:WIDTh? (Query Only)

Returns the pulse width in the pulse statistics. This command is valid when [DISPlay:PULSe:STATistics:PLOT](#) is set to TREND.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:WIDTh?
Arguments	None
Returns	<code><width_avg></code> , <code><width_min></code> , <code><width_max></code>

Where
 <width_avg>::=<NRF> is the average pulse width.
 <width_min>::=<NRF> is the minimum pulse width.
 <width_max>::=<NRF> is the maximum pulse width.
 Unit: Seconds.

Examples `READ:PULSE:STATISTICS:WIDTH?` might return
 4.636E-6, 4.630E-6, 4.643E-6 for the pulse width in the pulse statistics.

READ:PULSe:STATistics:X? (Query Only)

Returns the horizontal values of the trace data of the pulse statistics measurement selected by the `DISPlay:PULSe:SElect:RESult` command.

NOTE. Select the plot type (Trend, FFT, Time Trend or Histogram) using the `DISPlay:PULSe:STATistics:PLOT` command before executing this query.

Conditions Measurement views: Pulse statistics

Group Read commands

Syntax `READ:PULSe:STATistics:X?`

Arguments None

Returns `#<num_digit><num_byte><data1><data2>...data<n>`

Where
 <num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <data(n)> is the horizontal value of the statistics graph at the nth data point.
 The unit is trace number (Plot = Trend), Hz (Plot = FFT), second (Plot = Time Trend) or current measurement unit (Plot = Histogram).
 4-byte little endian floating-point format specified in IEEE 488.2.

Examples `READ:PULSE:STATISTICS:X?` might return `#264xxxx...` (64-byte data) for the statistics trace of the pulse width measurement when `DISPlay:PULSe:SElect:RESult` is set to `WIDTH`.

READ:PULSe:STATistics:XY? (Query Only)

Returns the horizontal and vertical values of the trace data of the pulse statistics measurement selected by the [DISPlay:PULSe:SElect:RESult](#) command.

NOTE. Select the plot type (Trend, FFT, Time Trend or Histogram) using the [DISPlay:PULSe:STATistics:PLOT](#) command before executing this query.

Conditions	Measurement views: Pulse statistics
Group	Read commands
Syntax	READ:PULSe:STATistics:XY?
Arguments	None
Returns	<p>#<num_digit><num_byte><data1><data2>...data<n></p> <p>Where</p> <ul style="list-style-type: none"> <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the horizontal value of the statistics graph at the nth data point. <data(n+1)> is the vertical value of the statistics graph at the nth data point. <p>For horizontal values, the unit is trace number (Plot = Trend), Hz (Plot = FFT), second (Plot = Time Trend) or current measurement unit (Plot = Histogram).</p> <p>For vertical values, the unit is current measurement unit (Plot = Trend or Time Trend), dB (Plot = FFT), count (Plot = Histogram)</p> <p>4-byte little endian floating-point format specified in IEEE 488.2.</p>
Examples	<p>READ:PULSE:STATISTICS:XY? might return #264xxxx... (64-byte data) for the statistics trace of the pulse width measurement when DISPlay:PULSe:SElect:RESult is set to WIDTH.</p>

READ:PULSe:STATistics[:Y]? (Query Only)

Returns the trace data of the pulse statistics measurement selected by the [DISPlay:PULSe:SElect:RESult](#) command.

NOTE. Select the plot type (Trend, FFT, Time Trend or Histogram) using the [DISPlay:PULSe:STATistics:PLOT](#) command before executing this query.

Conditions	Measurement views: Pulse statistics
Group	Fetch commands
Syntax	READ:PULSE:STATISTICS[:Y]?
Arguments	None
Returns	#<num_digit><num_byte><data(1)><data(2)>...<data(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <data(n)> is the amplitude at the n th data point. The unit is current measurement unit (Plot = Trend or Time Trend), dB (Plot = FFT), count or percent (Plot = Histogram) 4-byte little endian floating-point format specified in IEEE 488.2. The unit of power is selected by the [SENSe]:POWer:UNITs command.

READ:PULSE:TRACe:X? (Query Only)

Returns the time values of the pulse trace. Use the [DISPlay:PULSE:SElect:NUMBer](#) command to select the pulse, and the [DISPlay:PULSE:SElect:RESult](#) command to select the measurement result.

Conditions	Measurement views: Pulse trace
Group	Read commands
Syntax	READ:PULSE:TRACe:X?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><x(2)>...<x(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)> is the time in seconds at the n th data point,

4-byte little endian floating-point format specified in IEEE 488.2.

Examples `READ:PULSE:TRACE:X?` might return `#43204xxxx...` (3204-byte data) for the time values of the trace.

READ:PULSe:TRACe:XY? (Query Only)

Returns the horizontal (time) and vertical value pairs of the pulse trace. Use the [DISPlay:PULSe:SElect:NUMBer](#) command to select the pulse, and the [DISPlay:PULSe:SElect:RESult](#) command to select the measurement result.

Conditions Measurement views: Pulse trace

Group Read commands

Syntax `READ:PULSe:TRACe:XY?`

Arguments None

Returns `#<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)>...<x(n)><y(n)>`

Where

`<num_digit>` is the number of digits in `<num_byte>`.

`<num_byte>` is the number of bytes of data that follow.

`<x(n)><y(n)>` is the horizontal value (time in seconds) and vertical value pair at the n^{th} data point, 4-byte little endian floating-point format specified in IEEE 488.2.

The vertical unit depends on measurement results: Hz for frequency error and deviation, degrees for phase error and deviation, otherwise dBm. The vertical unit can be changed by the [\[SENSE\]:POWER:UNITs](#) command.

Examples `READ:PULSE:TRACE:XY?` might return `#43204xxxx...` (3204-byte data) for the horizontal (time) and vertical value pairs of the pulse trace.

READ:PULSe:TRACe[:Y]? (Query Only)

Returns the vertical values of the pulse trace. Use the [DISPlay:PULSe:SElect:NUMBer](#) command to select the pulse, and the [DISPlay:PULSe:SElect:RESult](#) command to select the measurement result.

Conditions	Measurement views: Pulse trace
Group	Read commands
Syntax	READ:PULSE:TRACE[:Y]?
Arguments	None
Returns	<p>#<num_digit><num_byte><y(1)><y(2)>...<y(n)></p> <p>Where</p> <p><num_digit> is the number of digits in <num_byte>.</p> <p><num_byte> is the number of bytes of data that follow.</p> <p><y(n)> is the vertical value of the pulse trace at the nth data point, 4-byte little endian floating-point format specified in IEEE 488.2.</p> <p>The unit depends on measurement results: Hz for frequency error and deviation, degrees for phase error and deviation, otherwise dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.</p>
Examples	READ:PULSE:TRACE:Y? might return #43204xxxx... (3204-byte data) for the vertical values of the pulse trace.

READ:SGRam? (Query Only)

Returns the spectrogram trace data. The line is selected using the [TRACE:SGRam:SElect:LINE](#) command.

Conditions	Measurement views: Spectrogram
Group	Read commands
Syntax	READ:SGRam?
Arguments	None
Returns	<p>#<num_digit><num_byte><data(1)><data(2)>...<data(n)></p> <p>Where</p> <p><num_digit> is the number of digits in <num_byte>.</p>

<num_byte> is the number of bytes of data that follow.
 <data(n)> is the trace data in dBm for the point n,
 4-byte little endian floating-point format specified in IEEE 488.2.
 The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples READ:SGRAM? might return #43204xxxx... (3204-byte data) for the spectrogram trace.

READ:SPECTrum:TRACe<x>? (Query Only)

Returns the trace data in the Spectrum measurement.

The parameter <x> = 1 to 5.

NOTE. TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.

Conditions Measurement views: Spectrum

Group Read commands

Syntax READ:SPECTrum:TRACe<x>?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the trace data in dBm for the point n,

4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples READ:SPECTRUM:TRACE1 might return #43204xxxx... (3204-byte data) for Trace 1 in the Spectrum measurement.

READ:SPURious:CARRier:POWer? (Query Only)

Returns the carrier power in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:CARRier:POWER?
Arguments	None
Returns	<NRF> Carrier power in dBm. The unit can be changed by the [SENSE]:POWER:UNITs command.
Examples	READ:SPURIOUS:CARRIER:POWER? might return 4.227, indicating that the carrier power is 4.227 dBm.

READ:SPURious:COUNT? (Query Only)

Returns the number of spurious signals in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:COUNT?
Arguments	None
Returns	<NRF> The spurious count.
Examples	READ:SPURIOUS:COUNT? might return 4, indicating that the spurious count is 4.

READ:SPURious:PASS? (Query Only)

Returns the pass/fail limit test result in the Spurious measurement.

Conditions	Measurement views: Spurious
-------------------	-----------------------------

Group	Read commands
Syntax	READ:SPURious:PASS?
Arguments	None
Returns	0 (fail) or 1 (pass).
Examples	READ:SPURIOUS:PASS? might return 1, indicating that the limit test was successful.

READ:SPURious:SPECTrum:X? (Query Only)

Returns the frequencies of the spectrum trace in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPECTrum:X?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><x(2)>...<x(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)> is the frequency (Hz) at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.
Examples	READ:SPURIOUS:SPECTRUM:X? might return #516020xxxx... (16020-byte data) for the frequencies of the spectrum trace in the Spurious measurement.

READ:SPURious:SPECTrum:XY? (Query Only)

Returns the frequency and amplitude pairs of the spectrum trace in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPECTrum:XY?
Arguments	None
Returns	#<num_digit><num_byte><x(1)><y(1)><x(2)><y(2)>...<x(n)><y(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <x(n)><y(n)> is the frequency (Hz) and amplitude (dBm) pair at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2. The amplitude unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	READ:SPURIOUS:SPECTRUM:XY? might return #516020xxxx... (16020-byte data) for the frequency and amplitude pairs of the spectrum trace in the Spurious measurement.

READ:SPURious:SPECTrum[:Y]? (Query Only)

Returns the amplitudes of the spectrum trace in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPECTrum[:Y]?
Related Commands	READ:SPURious:SPECTrum:X?
Arguments	None
Returns	#<num_digit><num_byte><y(1)><y(2)>...<y(n)> Where

<num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <y(n)> is the amplitude (dBm) at the nth data point,
 4-byte little endian floating-point format specified in IEEE 488.2.
 The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `READ:SPURIOUS:SPECTRUM:Y` might return `#516020xxxx...` (16020-byte data) for the amplitudes of the spectrum trace in the Spurious measurement.

READ:SPURious:SPUR<x>:AMPLitude:ABSolute? (Query Only)

Returns the absolute amplitude of the specified spurious signal in the Spurious measurement.

Conditions Measurement views: Spurious

Group Read commands

Syntax `READ:SPURious:SPUR<x>:AMPLitude:ABSolute?`

Arguments None

Returns <NRf> Absolute amplitude of the specified spurious in dBm.
 The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples `READ:SPURIOUS:SPUR1:AMPLITUDE:ABSOLUTE?` might return `-19.782`, indicating that the absolute amplitude of Spurious #1 is -19.782 dBm.

READ:SPURious:SPUR<x>:AMPLitude:RELative? (Query Only)

Returns the relative amplitude of the specified spurious signal in the Spurious measurement.

Conditions Measurement views: Spurious

Group Read commands

Syntax `READ:SPURious:SPUR<x>:AMPLitude:RELative?`

Arguments	None
Returns	<NRF> Relative amplitude of the specified spurious signal in dB. Use the [SENSe]:SPURious:REference command to set the power reference.
Examples	READ:SPURIOUS:SPUR1:AMPLITUDE:RELATIVE? might return -9.782, indicating that the relative amplitude of Spurious #1 is -9.782 dB.

READ:SPURious:SPUR<x>:FREQUENCY:ABSolute? (Query Only)

Returns the absolute frequency of the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPUR<x>:FREQUENCY:ABSolute?
Arguments	None
Returns	<NRF> Absolute frequency of the spurious signal in Hz.
Examples	READ:SPURIOUS:SPUR1:FREQUENCY:ABSOLUTE? might return 2.235E+9, indicating that the absolute frequency of Spurious #1 is 2.235 GHz.

READ:SPURious:SPUR<x>:FREQUENCY:RELative? (Query Only)

Returns the relative frequency of the specified spurious signal to the carrier in the Spurious measurement. This command is valid when [\[SENSe\]:SPURious:REference](#) is set to CARRIER.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPUR<x>:FREQUENCY:RELative?

Arguments	None
Returns	<Nrf> Relative frequency of the spurious signal to the carrier in Hz.
Examples	READ:SPURIOUS:SPUR1:FREQUENCY:RELATIVE? might return 3.634E+6, indicating that the relative frequency of Spurious #1 is 3.634 MHz.

READ:SPURious:SPUR<x>:LIMit:ABSolute? (Query Only)

Returns the absolute amplitude of the limit for the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPUR<x>:LIMit:ABSolute?
Arguments	None
Returns	<Nrf> Absolute amplitude of the limit for the specified spurious signal in dBm. The unit can be changed by the [SENSe]:POWer:UNITs command.
Examples	READ:SPURIOUS:SPUR1:LIMIT:ABSOLUTE? might return -50.0, indicating that the absolute amplitude of the limit for Spurious #1 is -50 dBm.

READ:SPURious:SPUR<x>:LIMit:RELative? (Query Only)

Returns the relative amplitude of the limit for the specified spurious signal in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPUR<x>:LIMit:RELative?

Arguments	None
Returns	<NRF> Relative amplitude of the limit for the specified spurious signal in dB. Use the [SENSe]:SPURious:REference command to set the power reference.
Examples	READ:SPURIOUS:SPUR1:LIMIT:RELATIVE? might return -10.0, indicating that the relative amplitude of the limit for Spurious #1 is -10 dB.

READ:SPURious:SPUR<x>:LIMit:VIOLation? (Query Only)

Returns whether the specified spurious signal exceeds the limit or not.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPUR<x>:LIMit:VIOLation?
Arguments	None
Returns	0 (under the limit) or 1 (over the limit).
Examples	READ:SPURIOUS:SPUR1:LIMIT:VIOLATION? might return 1, indicating that Spurious #1 exceeds the limit.

READ:SPURious:SPUR<x>:RANGe? (Query Only)

Returns the frequency range in which the specified spurious signal occurred.

Conditions	Measurement views: Spurious
Group	Read commands
Syntax	READ:SPURious:SPUR<x>:RANGe?
Arguments	None

Returns <string> "A" to "T" representing Range A to T, respectively.

Examples READ:SPURIOUS:SPUR1:RANGE? might return "E", indicating that Spurious #1 is in Range E.

READ:SQUALity:FREQUency:DEViation? (Query Only)

Returns the frequency deviation in the signal quality measurement.

This command is valid when [SENSe]:DDEMod:MODulation:TYPE is set to C4FM, FSK2, FSK4, FSK8, or FSK16.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUALity:FREQUency:DEViation?

Arguments None

Returns <Nrf> Frequency deviation in Hz.

Examples READ:SQUALITY:FREQUENCY:DEVIATION? might return 12.68E+3, indicating the frequency deviation is 12.68 kHz.

READ:SQUALity:FREQUency:DEViation:TABLE? (Query Only)

Returns the number of columns and the values in the frequency deviation table for a signal quality measurement.

This command is valid when [SENSe]:DDEMod:MODulation:TYPE is set to C4FM, FSK2, FSK4, FSK8, or FSK16.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUALity:FREQUency:DEViation:TABLE?

Arguments None

Returns <Dev_Num>, {<Freq_dev_Max>, <Freq_dev_Min>, <Freq_dev_Avg>}

Where

<Dev_Num> ::= <NR1> is the number of columns in the frequency deviation table.
= 2 (2FSK), 4 (4FSK, C4FM), 8 (8FSK), or 16 (16FSK)

<Freq_dev_Max> ::= <NRf> is the maximum frequency deviation in Hz.

<Freq_dev_Min> ::= <NRf> is the minimum frequency deviation in Hz.

<Freq_dev_Avg> ::= <NRf> is the average frequency deviation in Hz.

The dataset <Freq_dev_Max>, <Freq_dev_Min>, <Freq_dev_Avg> is returned for each symbol in ascending order of its level (for example, in order of symbol -3, -1, +1, and +3 for 4FSK).

Examples READ:SQUALITY:FREQUENCY:DEVIATION:TABLE? might return 2, 1.257E+3, 1.039E+3, 1.162E+3, 1.586E+3, 1.298E+3, 1.425E+3 for the frequency signal, populating the results table as follows.

Deviations	-1	+1
Maximum	1.257 kHz	1.586 kHz
Minimum	1.039 kHz	1.298 kHz
Average	1.162 kHz	1.425 kHz

READ:SQUALITY:FREQUENCY:ERROR? (Query Only)

Returns the frequency error in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUALITY:FREQUENCY:ERROR?

Arguments None

Returns <NRf> Frequency error in Hz.

Examples READ:SQUALITY:FREQUENCY:ERROR? might return 612.043E+3, indicating that the frequency error is 612.043 kHz.

READ:SQUALity:GAIN:IMBalance? (Query Only)

Returns the gain imbalance in the signal quality measurement.

Conditions	Measurement views: Signal quality
Group	Read commands
Syntax	READ:SQUALity:GAIN:IMBalance?
Arguments	None
Returns	<NRf> Gain imbalance in dB.
Examples	READ:SQUALITY:GAIN:IMBALANCE? might return $-57.746E-3$, indicating that the gain imbalance is -0.057746 dB.

READ:SQUALity:ORIGIN:OFFSet? (Query Only)

Returns the origin offset in the signal quality measurement.

Conditions	Measurement views: Signal quality
Group	Read commands
Syntax	READ:SQUALity:ORIGIN:OFFSet?
Arguments	None
Returns	<NRf> Origin offset in dB.
Examples	READ:SQUALITY:ORIGIN:OFFSET? might return -44.968 , indicating that the origin offset is -44.968 dB.

READ:SQUALity:PEAK:EVM? (Query Only)

Returns the peak EVM (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUALity:PEAK:EVM?

Arguments None

Returns <NRF> Peak EVM in percent (%).

Examples READ:SQUALITY:PEAK:EVM? might return 4.276, indicating that the peak EVM is 4.276%.

READ:SQUALity:PEAK:EVM:DB? (Query Only)

Returns the peak EVM (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUALity:PEAK:EVM:DB?

Arguments None

Returns <NRF> Peak EVM in dB.

Examples READ:SQUALITY:PEAK:EVM:DB? might return -27.358, indicating that the peak EVM is -27.358 dB.

READ:SQUALity:PEAK:EVM:DB:OFFSet? (Query Only)

Returns the peak offset EVM (dB) in the signal quality measurement.

This command is valid when `[SENSe]:DDEMod:MODulation:TYPE` is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Read commands
Syntax	<code>READ:SQUALity:PEAK:EVM:DB:OFFSet?</code>
Arguments	None
Returns	<NRF> Peak offset EVM in dB.
Examples	<code>READ:SQUALITY:PEAK:EVM:DB:OFFSET?</code> might return <code>-37.624</code> , indicating the peak offset EVM is <code>-37.624</code> dB.

READ:SQUALity:PEAK:EVM:LOCation? (Query Only)

Returns the time at which the EVM is peak.

Conditions	Measurement views: Signal quality
Group	Read commands
Syntax	<code>READ:SQUALity:PEAK:EVM:LOCation?</code>
Arguments	None
Returns	<NRF> The time in symbol number at which the EVM is peak. The unit can be changed by the <code>[SENSe]:DDEMod:TIME:UNITs</code> command.
Examples	<code>READ:SQUALITY:PEAK:EVM:LOCATION?</code> might return <code>68.000</code> , indicating that the EVM is peak at symbol #68.000.

READ:SQUality:PEAK:EVM:LOCation:OFFSet? (Query Only)

Returns the time at which the offset EVM is peak.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Read commands
Syntax	READ:SQUality:PEAK:EVM:LOCation:OFFSet?
Arguments	None
Returns	<NRf> The time in symbol number at which the offset EVM is peak. The unit can be changed by the [SENSe]:DDEMod:TIME:UNITs command.
Examples	READ:SQUALITY:PEAK:EVM:LOCATION:OFFSET? might return 123.00, indicating that the offset EVM is peak at symbol #123.

READ:SQUality:PEAK:EVM:OFFSet? (Query Only)

Returns the peak offset EVM (%) in the signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions	Measurement views: Signal quality
Group	Read commands
Syntax	READ:SQUality:PEAK:EVM:OFFSet?
Arguments	None
Returns	<NRf> Peak offset EVM in percent (%).

Examples READ: SQUALITY: PEAK: EVM: OFFSET? might return 1.298, indicating the peak offset EVM is 1.298%.

READ: SQUALITY: PEAK: FERROR? (Query Only)

Returns the peak FSK error in the signal quality measurement.

This command is valid when [SENSe]: DDEMod: MODulation: TYPE is set to FSK2, FSK4, FSK8, or FSK16.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ: SQUALITY: PEAK: FERROR?

Arguments None

Returns <NRf> Peak FSK error in percent (%).

Examples READ: SQUALITY: PEAK: FERROR? might return 9.136, indicating the peak FSK error is 9.136%.

READ: SQUALITY: PEAK: MERROR? (Query Only)

Returns the peak magnitude error (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ: SQUALITY: PEAK: MERROR?

Arguments None

Returns <NRf> Peak magnitude error in percent (%).

Examples `READ:SQUALITY:PEAK:MERROR?` might return 3.595, indicating that the peak magnitude error is 3.595%.

READ:SQUALITY:PEAK:MERROR:DB? (Query Only)

Returns the peak magnitude error (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax `READ:SQUALITY:PEAK:MERROR:DB?`

Arguments None

Returns <NRF> Peak magnitude error in dB.

Examples `READ:SQUALITY:PEAK:MERROR:DB?` might return -28.583, indicating that the magnitude error is -28.583 dB.

READ:SQUALITY:PEAK:MERROR:LOCATION? (Query Only)

Returns the time at which the magnitude error is peak.

Conditions Measurement views: Signal quality

Group Read commands

Syntax `READ:SQUALITY:PEAK:MERROR:LOCATION?`

Arguments None

Returns <NRF> The time in symbol number at which the magnitude error is peak.
The unit can be changed by the `[SENSE]:DDEMod:TIME:UNITs` command.

Examples `READ:SQUALITY:PEAK:MERROR:LOCATION?` might return `68.000`, indicating that the magnitude error is peak at symbol #68.

`READ:SQUALITY:PEAK:PERROR?` (Query Only)

Returns the peak phase error in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax `READ:SQUALITY:PEAK:PERROR?`

Arguments None

Returns `<NRf>` Peak phase error in degrees.

Examples `READ:SQUALITY:PEAK:PERROR?` might return `1.907`, indicating that the peak phase error is `1.907 °`.

`READ:SQUALITY:PEAK:PERROR:LOCATION?` (Query Only)

Returns the time at which the phase error is peak.

Conditions Measurement views: Signal quality

Group Read commands

Syntax `READ:SQUALITY:PEAK:PERROR:LOCATION?`

Arguments None

Returns `<NRf>` The time in symbol number at which the phase error is peak. The unit can be changed by the `[SENSE]:DDEMod:TIME:UNITS` command.

Examples READ:QUALITY:PEAK:ERROR:LOCATION? might return 68.000, indicating that the phase error is peak at symbol #68.

READ:QUALITY:QUADRATURE:ERROR? (Query Only)

Returns the quadrature error in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:QUALITY:QUADRATURE:ERROR?

Arguments None

Returns <NRf> Quadrature error in degrees.

Examples READ:QUALITY:QUADRATURE:ERROR? might return -14.264E-3, indicating that the quadrature error is -0.014264°.

READ:QUALITY:RHO? (Query Only)

Returns the ρ (waveform quality) value in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:QUALITY:RHO?

Arguments None

Returns <NRf> ρ value.

Examples READ:QUALITY:RHO? might return 998.703E-3, indicating that ρ is 0.998703.

READ:SQUality:RMS:EVM? (Query Only)

Returns the RMS EVM (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUality:RMS:EVM?

Arguments None

Returns <NRf> RMS EVM in percent (%).

Examples READ:SQUALITY:RMS:EVM? might return 2.417, indicating that the RMS EVM is 2.417%.

READ:SQUality:RMS:EVM:DB? (Query Only)

Returns the RMS EVM (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUality:RMS:EVM:DB?

Arguments None

Returns <NRf> RMS EVM in dB.

Examples READ:SQUALITY:RMS:EVM:DB? might return -32.356, indicating that the RMS EVM is -32.356 dB.

READ:SQUALity:RMS:EVM:DB:OFFSet? (Query Only)

Returns the RMS offset EVM (dB) in the signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUALity:RMS:EVM:DB:OFFSet?

Arguments None

Returns <NRF> RMS offset EVM in dB.

Examples READ:SQUALITY:RMS:EVM:DB:OFFSET? might return -41.276, indicating the RMS offset EVM is -41.276 dB.

READ:SQUALity:RMS:EVM:OFFSet? (Query Only)

Returns the RMS offset EVM (%) in the signal quality measurement.

This command is valid when [\[SENSe\]:DDEMod:MODulation:TYPE](#) is set to OQPSK or SOQPSK.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUALity:RMS:EVM:OFFSet?

Arguments None

Returns <NRF> RMS offset EVM in percent (%).

Examples READ:QUALITY:RMS:EVM:OFFSET? might return 0.783, indicating the RMS offset EVM is 0.783%.

READ:QUALITY:RMS:FERROR? (Query Only)

Returns the RMS FSK error in the signal quality measurement.

This command is valid when [SENSe]:DDEMod:MODulation:TYPE is set to FSK2, FSK4, FSK8, or FSK16.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:QUALITY:RMS:FERROR?

Arguments None

Returns <NRf> RMS FSK error in percent (%).

Examples READ:QUALITY:RMS:FERROR? might return 8.67, indicating the RMS FSK error is 8.67%.

READ:QUALITY:RMS:MER:DB? (Query Only)

Returns the RMS MER (Modulation Error Ratio) in dB in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:QUALITY:RMS:MER:DB?

Arguments None

Returns <NRf> RMS MER in dB.

Examples `READ:SQUALITY:RMS:MERRor:DB?` might return `27.394`, indicating that the RMS MER is 27.394 dB.

READ:SQUALity:RMS:MERRor? (Query Only)

Returns the RMS magnitude error (%) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax `READ:SQUALity:RMS:MERRor?`

Arguments None

Returns <NRF> RMS magnitude error in percent (%).

Examples `READ:SQUALITY:RMS:MERROR?` might return `1.837`, indicating that the RMS magnitude error is 1.837%.

READ:SQUALity:RMS:MERRor:DB? (Query Only)

Returns the RMS magnitude error (dB) in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax `READ:SQUALity:RMS:MERRor:DB?`

Arguments None

Returns <NRF> RMS magnitude error in dB.

Examples `READ:SQUALITY:RMS:MERROR:DB?` might return `-34.706`, indicating that the magnitude error is -34.706 dB.

READ:SQUality:RMS:PERRor? (Query Only)

Returns the RMS phase error in the signal quality measurement.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUality:RMS:PERRor?

Arguments None

Returns <NRf> RMS phase error in degrees.

Examples READ:SQUALITY:RMS:PERROR? might return 893.472E-3, indicating that the RMS phase error is 0.893472 °.

READ:SQUality:SYMBol:LENGth? (Query Only)

Returns the number of analyzed symbols.

Conditions Measurement views: Signal quality

Group Read commands

Syntax READ:SQUality:SYMBol:LENGth?

Related Commands

Returns <NR1> indicates the length of the synch word in symbols.

Examples READ:SQUALITY:SYMBOL:LENGTH? might return 3, indicating the length is three symbols.

READ:SQUality:SYMBol:RATE? (Query Only)

Returns the value of the calculated symbol rate in Hz.

Conditions	Measurement views: Signal quality It is valid when the modulation type is 2 4 8 16FSK and [:SENSe]:DDEMod:SYMBOL:RATE:SEARCh is ON.
Group	Read commands
Syntax	READ:SQUALity:SYMBOL:RATE?
Related Commands	[SENSe]:DDEMod:SYMBOL:RATE:SEARCh
Returns	<NRf> is the calculated symbol rate in Hz.
Examples	READ:SQUALITY:SYMBOL:RATE? might return 95.24E+3, indicating the calculated symbol rate is 95.24 kHz.

READ:SQUALity:SYMBOL:RATE:ERRor? (Query Only)

Returns the value of the symbol rate error in percent (%).

Conditions	Measurement views: Signal quality It is valid when the modulation type is 2 4 8 16FSK and [:SENSe]:DDEMod:SYMBOL:RATE:SEARCh is ON.
Group	Read commands
Syntax	READ:SQUALity:SYMBOL:RATE:ERRor?
Related Commands	[SENSe]:DDEMod:SYMBOL:RATE:SEARCh
Returns	<NRf> is the symbol error percent (%).
Examples	READ:SQUALITY:SYMBOL:RATE:ERROR? might return -0.002, indicating that the symbol rate error is -0.002%.

READ:TDIagram:FERRor? (Query Only)

Returns the frequency error in the trellis diagram measurement.

Conditions	Measurement views: Trellis diagram
Group	Read commands
Syntax	READ:TDIagram:FERRor?
Arguments	None
Returns	<freq_error> ::= <NRF> is the frequency error in Hz.
Examples	READ:TDIAGRAM:FERROR? might return -10.7E+3, indicating the frequency error is -10.7 kHz.

READ:TDIagram:TRACe? (Query Only)

Returns the Trellis diagram trace data.

Conditions	Measurement views: Trellis diagram
Group	Read commands
Syntax	READ:TDIagram:TRACe?
Arguments	None
Returns	#<num_digit><num_byte><Y(1)><X(1)><Y(2)><X(2)>...<Y(n)><X(n)> Where <num_digit> is the number of digits in <num_byte>. <num_byte> is the number of bytes of data that follow. <Y(n)><X(n)> is the phase in degrees and the time in symbols pair at the n th data point, 4-byte little endian floating-point format specified in IEEE 488.2.

Examples READ:TDIAGRAM:TRACE? might return #3160xxxx... (160-byte data) for the Trellis diagram trace.

READ:TOVerview? (Query Only)

Returns the trace data in the time overview.

Conditions Measurement views: Time overview

Group Read commands

Syntax READ:TOVerview?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the trace data in dBm for the point n,

4-byte little endian floating-point format specified in IEEE 488.2.

The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) command.

Examples READ:TOVERVIEW? might return #43204xxxx... (3204-byte data) for the trace in the time overview.

*RST (No Query Form)

Returns the instrument settings to the factory defaults ((See page 3-1, *Factory Initialization Settings*.)

The *RST command does not alter the following

- The state of the GPIB interface.
- The selected GPIB address of the analyzer.
- Alignment data that affect device specifications.
- The Output Queue.
- The Service Request Enable Register setting.
- The Standard Event Status Enable Register setting.
- The Power-on status clear flag setting.
- Stored settings.

NOTE. Execution of the **RST* command is not complete until all changes from resetting the instrument are completed. Following commands and queries will not be executed until these actions are completed.

Conditions Measurement views: All

Group IEEE common commands

Syntax *RST

Related Commands [*CLS](#)

Arguments None

Examples *RST returns the instrument settings to the factory defaults.

[SENSe]:ACPower:AVERage

Sets or queries how to average waveform in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax [SENSe]:ACPower:AVERage { OFF | TIME | FREquency }
[SENSe]:ACPower:AVERage?

Arguments OFF disables averaging.
TIME averages waveform using time samples.
FREquency averages waveform using frequency samples.

Examples SENSE:ACPOWER:AVERAGE TIME averages waveform using time samples.

[SENSe]:ACPower:AVERage:COUNT

Sets or queries the number of traces for averaging in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax [SENSe]:ACPower:AVERage:COUNT <number>
[SENSe]:ACPower:AVERage:COUNT?

Arguments <number>::=<NR1> specifies the average count. Range: 2 to 10000.

Examples SENSE:ACPOWER:AVERAGE:COUNT 64 sets the average count to 64.

[SENSe]:ACPower:{BANDwidth|BWIDth}[:RESolution]

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [SENSe]:ACPower:{BANDwidth|BWIDth}[:RESolution]:AUTO OFF.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax [SENSe]:ACPower:{BANDwidth|BWIDth}[:RESolution] <value>
[SENSe]:ACPower:{BANDwidth|BWIDth}[:RESolution]?

Related Commands `[SENSE]:ACPower:{BANDwidth|BWIDth}[:RESolution]:AUTO`

Arguments `<value>::=<NRf>` specifies the RBW. Range: 100 Hz to 5 MHz.

Examples `SENSE:ACPOWER:BANDWIDTH:RESOLUTION 200kHz` sets the RBW to 200 kHz.

`[SENSE]:ACPower:{BANDwidth|BWIDth}[:RESolution]:ACTual? (Query Only)`

Queries the actual resolution bandwidth (RBW) in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax `[SENSE]:ACPower:{BANDwidth|BWIDth}[:RESolution]:ACTual?`

Arguments None

Returns `<NRf>` The actual RBW in Hz.

Examples `SENSE:ACPOWER:BANDWIDTH:RESOLUTION:ACTUAL?` might return `299.624E+3`, indicating that the actual RBW is 299.624 kHz.

`[SENSE]:ACPower:{BANDwidth|BWIDth}[:RESolution]:AUTO`

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax `[SENSE]:ACPower:{BANDwidth|BWIDth}[:RESolution]:AUTO { OFF | ON | 0 | 1 }`
`[SENSE]:ACPower:{BANDwidth|BWIDth}[:RESolution]:AUTO?`

Arguments OFF or 0 specifies that the RBW is set manually using the `[SENSe]:ACPower:{BANDwidth|BWIDth}:RESolution` command.
ON or 1 specifies that the RBW is set automatically.

Examples `SENSE:ACPOWER:BANDWIDTH:AUTO ON` sets the RBW automatically.

`[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo`

Sets or queries the video bandwidth (VBW). Programming a specified VBW sets `[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo:STATE` OFF.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax `[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo <value>`
`[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo?`

Related Commands `[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo:STATE`

Arguments `<value>::=<NRF>` specifies the VBW.
Range: Current RBW/10⁴ (1 Hz minimum) to Current RBW.

Examples `SENSE:ACPOWER:BANDWIDTH:VIDEO 200kHz` sets the VBW to 200 kHz.

`[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo:STATE`

Determines whether to enable or disable the video bandwidth (VBW) in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax `[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo:STATE { OFF | ON | 0 | 1 }`
`[SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo:STATE?`

- Arguments** OFF or 0 disables the VBW.
ON or 1 enables the VBW.
- Examples** SENSE:ACPOWER:BANDWIDTH:VIDEO:STATE ON enables the VBW.

[SENSe]:ACPower:CHANnel:{BANDwidth|BWIDth}

Sets or queries frequency bandwidth of each channel (all share the same value) in the Channel power and ACPR measurement.

- Conditions** Measurement views: Channel power and ACPR
- Group** Sense commands
- Syntax** [SENSe]:ACPower:CHANnel:{BANDwidth|BWIDth} <value>
[SENSe]:ACPower:CHANnel:{BANDwidth|BWIDth}?
- Arguments** <value>::=<Nrf> specifies the channel bandwidth. Range: 1 Hz to full span.
- Examples** SENSE:ACPOWER:CHANNEL:BANDWIDTH 1.5MHZ sets the channel bandwidth to 1.5 MHz.

[SENSe]:ACPower:CHANnel:FILTer

Sets or queries the adjacent channel filter in the Channel power and ACPR measurement.

- Conditions** Measurement views: Channel power and ACPR
- Group** Sense commands
- Syntax** [SENSe]:ACPower:CHANnel:FILTer { RRCosine | NONE }
[SENSe]:ACPower:CHANnel:FILTer?
- Arguments** RRCosine uses the Root-Raised Cosine filter.
NONE uses no filter.

Examples `SENSE:ACPOWER:CHANNEL:FILTER RRCosine` uses the Root-Raised Cosine filter for the Channel power and ACPR measurement.

[SENSe]:ACPower:CHANnel:PAIRs

Sets or queries the number of adjacent channel pairs (upper and lower) in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax `[SENSe]:ACPower:CHANnel:PAIRs <number>`
`[SENSe]:ACPower:CHANnel:PAIRs?`

Arguments `<number>::=<NR1>` specifies the number of adjacent pairs. Range: 0 to 50.

Examples `SENSE:ACPOWER:CHANNEL:PAIRS 5` sets five adjacent channel pairs.

[SENSe]:ACPower:CHANnel:SPACing

Sets or queries frequency difference between centers of each channel in the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax `[SENSe]:ACPower:CHANnel:SPACing <value>`
`[SENSe]:ACPower:CHANnel:SPACing?`

Arguments `<value>::=<NRf>` specifies the channel-to-channel spacing.
 Range: 1 Hz to 1 GHz.

Examples `SENSE:ACPOWER:CHANNEL:SPACING 5MHZ` sets the channel-to-channel spacing to 5 MHz.

[SENSe]:ACPower:CHIPrate

Sets or queries the chip rate when [SENSe]:ACPower:CHANnel:FILTer is set to RRCosine (Root Raised Cosine).

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax [SENSe]:ACPower:CHIPrate <value>
[SENSe]:ACPower:CHIPrate?

Related Commands [\[SENSe\]:ACPower:CHANnel:FILTer](#)

Arguments <value>::=<Nrf> specifies the chip rate. Range: 100 Hz to 105 MHz.

Examples SENSE:ACPOWER:CHIPRATE 5kHz sets the chip rate to 5 kHz.

[SENSe]:ACPower:CLEar:RESuLts (No Query Form)

Restarts the average trace.

Conditions Measurement views: Channel power and ACPR

Group Sense commands

Syntax [SENSe]:ACPower:CLEar:RESuLts

Arguments None

Examples SENSE:ACPOWER:CLEAR:RESULTS restarts the average trace.

[SENSe]:ACPower:FREQuency

Sets or queries the center frequency in the Channel power and ACPR measurement.

Conditions	Measurement views: Channel power and ACPR
Group	Sense commands
Syntax	[SENSe]:ACPower:FREQUENCY <value> [SENSe]:ACPower:FREQUENCY?
Arguments	<value>::=<Nrf> specifies the center frequency. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:ACPOWER:FREQUENCY 2.35GHZ sets the center frequency to 2.35 GHz.

[SENSe]:ACPower:FREQUENCY:STEP

Sets or queries the frequency step size in the Channel power and ACPR measurement. Programming a specified step size sets [SENSe]:ACPower:FREQUENCY:STEP:AUTO OFF.

Conditions	Measurement views: Channel power and ACPR
Group	Sense commands
Syntax	[SENSe]:ACPower:FREQUENCY:STEP <value> [SENSe]:ACPower:FREQUENCY:STEP?
Related Commands	[SENSe]:ACPower:FREQUENCY:STEP:AUTO
Arguments	<value>::=<Nrf> specifies the frequency step size. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:ACPOWER:FREQUENCY:STEP 1kHz sets the frequency step size to 1 kHz.

[SENSe]:ACPower:FREQUENCY:STEP:AUTO

Determines whether to set the frequency step size automatically or manually in the Channel power and ACPR measurement.

Conditions	Measurement views: Channel power and ACPR
Group	Sense commands
Syntax	[SENSE]:ACPower:FREQUENCY:STEP:AUTO { OFF ON 0 1 } [SENSE]:ACPower:FREQUENCY:STEP:AUTO?
Arguments	OFF or 0 specifies that the frequency step size is set manually using the [SENSE]:ACPower:FREQUENCY:STEP command. ON or 1 specifies that the frequency step size is set automatically.
Examples	SENSE:ACPOWER:FREQUENCY:STEP:AUTO ON specifies that the frequency step size is set automatically.

[SENSE]:ACPower:NFLoor:STATE

Determines whether to enable or disable the correction for noise floor.

Conditions	Measurement views: Channel power and ACPR
Group	Sense commands
Syntax	[SENSE]:ACPower:NFLoor:STATE { OFF ON 0 1 } [SENSE]:ACPower:NFLoor:STATE?
Arguments	OFF or 0 disables the correction for noise floor. ON or 1 enables the correction for noise floor.
Examples	SENSE:ACPOWER:NFLOOR:STATE ON enables the correction for noise floor.

[SENSE]:ACPower:OPTimize:SPAN

Sets or queries the optimization method in the Channel power and ACPR measurement.

Conditions	Measurement views: Channel power and ACPR
-------------------	---

Group	Sense commands
Syntax	[SENSe]:ACPower:OPTimize:SPAN { RTBandwidth DRANge } [SENSe]:ACPower:OPTimize:SPAN?
Arguments	RTBandwidth optimizes the measurement for real-time bandwidth. DRANge optimizes the measurement for dynamic range.
Examples	SENSE:ACPOWER:OPTIMIZE:SPAN RTBandwidth optimizes the measurement for real-time bandwidth.

[SENSe]:ACPower:POINTs:COUNT

Sets or queries the number of points used for the trace in the Channel Power and ACPR measurement.

Conditions	Measurement views: Channel power and ACPR
Group	Sense commands
Syntax	[SENSe]:ACPower:POINTs:COUNT { P801 P2401 P4001 P8001 P10801 } [SENSe]:ACPower:POINTs:COUNT?
Arguments	RTBandwidth optimizes the measurement for real-time bandwidth. DRANge optimizes the measurement for dynamic range.
Examples	SENSE:ACPOWER:POINTS:COUNT P4001 sets the number of points used in the trace of the Channel Power and ACPR display to 4001.

[SENSe]:ACPower:RRCRolloff

Sets or queries the filter parameter (roll-off ratio) for the Root Raised Cosine filter.

Conditions	Measurement views: Channel power and ACPR
Group	Sense commands

Syntax [SENSE]:ACPower:RRCRolloff <value>
[SENSE]:ACPower:RRCRolloff?

Related Commands [\[SENSE\]:ACPower:CHANnel:FILTer](#)

Arguments <value>::=<Nrf> specifies the filter parameter.
Range: 0.0001 to 1 in 0.0001 steps.

Examples SENSE:ACPOWER:RRCROLLOFF 0.3 sets the filter parameter to 0.3.

[SENSE]:ACQuisition:{BANDwidth|BWIDth}

Sets or queries the acquisition bandwidth (frequency range of the acquisition) when [\[SENSE\]:ACQuisition:MODE](#) is set to SAMPlEs or LENGth.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:ACQuisition:{BANDwidth|BWIDth} <value>
[SENSE]:ACQuisition:{BANDwidth|BWIDth}?

Arguments <value>::=<Nrf> specifies the acquisition bandwidth.
Range: 1 MHz to 40 MHz (Standard) / 110 MHz (Option 110).

Examples SENSE:ACQUISITION:BANDWIDTH 30MHZ sets the acquisition bandwidth to 30 MHz.

[SENSE]:ACQuisition:FFrame:ACTual? (Query Only)

Queries the actual number of Fast Frames.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:ACQuisition:FFrame:ACTual?

Arguments	None
Returns	<NR1> The actual number of Fast Frames.
Examples	SENSE:ACQUISITION:FFRAME:ACTUAL? might return 178, indicating that the actual number of Fast Frames is 178.

[SENSe]:ACQuisition:FFRame:LIMit

Sets or queries the limit number of Fast Frames.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:ACQuisition:FFRame:LIMit [SENSe]:ACQuisition:FFRame:LIMit?
Arguments	<value>::=<NR1> specifies the fast frame limit. Range: 1 to 65535 frames.
Examples	SENSE:ACQUISITION:FFRAME:LIMIT 500 sets the Fast Frame limit to 500.

[SENSe]:ACQuisition:FFRame:STATe

Determines whether to enable or disable the Fast Frame.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:ACQuisition:FFRame:STATe { OFF ON 0 1 } [SENSe]:ACQuisition:FFRame:STATe?
Arguments	OFF or 0 disables the Fast Frame. ON or 1 enables the Fast Frame.

Examples `SENSE:ACQUISITION:FFRAME:STATE ON` enables the Fast Frame.

[SENSe]:ACQuisition:MEMory:AVAIlable:SAMPles? (Query Only)

Returns the amount of acquisition memory available in the instrument.

Conditions Measurement views: All

Group Sense commands

Syntax `[SENSe]:ACQuisition:MEMory:AVAIlable:SAMPles?`

Arguments None

Returns `<NRf>` The amount of acquisition memory available in samples.

Examples `SENSE:ACQUISITION:MEMORY:AVAILABLE:SAMPLES?` might return `999.424E+3`, indicating that 999424 samples are available.

[SENSe]:ACQuisition:MEMory:CAPacity[:TIME]? (Query Only)

Returns the acquisition memory capacity (maximum period of time that can be acquired with the acquisition memory).

Conditions Measurement views: All

Group Sense commands

Syntax `[SENSe]:ACQuisition:MEMory:CAPacity[:TIME]?`

Arguments None

Returns `<NRf>` The acquisition memory capacity in seconds.

Examples `SENSE:ACQUISITION:MEMORY:CAPACITY:TIME?` might return `26.651E-3`, indicating that 26.651 ms can be acquired.

[SENSe]:ACQuisition:MEMory:USED[:PERCent]? (Query Only)

Returns the percentage of the capacity used based on the current settings.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:ACQuisition:MEMory:USED[:PERCent]?
Arguments	None
Returns	<NRF> The percentage of the capacity used.
Examples	SENSe:ACQuisition:MEMory:USED:PERCENT? might return 50.0, indicating that 50% is used.

[SENSe]:ACQuisition:MODE

Sets or queries the acquisition mode (how to determine the sampling parameters of acquisition bandwidth, samples, and length).

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:ACQuisition:MODE { AUTO SAMPlEs LENGth } [SENSe]:ACQuisition:MODE?
Related Commands	[SENSe]:ACQuisition:{BANDwidth BWIDTH} , [SENSe]:ACQuisition:SAMPlEs , [SENSe]:ACQuisition:SEConds
Arguments	AUTO sets the all sampling parameters automatically. SAMPlEs sets the acquisition bandwidth and samples manually, using the [SENSe]:ACQuisition:{BANDwidth BWIDTH} and :SAMPlEs commands. LENGth sets the acquisition bandwidth and length manually, using the [SENSe]:ACQuisition:{BANDwidth BWIDTH} and :SEConds commands.

Examples SENSE:ACQUISITION:MODE AUTO sets the all sampling parameters automatically.

[SENSE]:ACQuisition:SAMPles

Sets or queries the acquisition samples (number of samples acquired over the acquisition time) when [SENSE]:ACQuisition:MODE is set to SAMPles.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:ACQuisition:SAMPles <value>
[SENSE]:ACQuisition:SAMPles?

Arguments <value>::=<NR1> specifies the acquisition samples. Range: 2 to 1 G samples.

Examples SENSE:ACQUISITION:SAMPLES 1114 sets the acquisition samples to 1114.

[SENSE]:ACQuisition:SEConds

Sets or queries the acquisition length (time over which the acquisition occurs) when [SENSE]:ACQuisition:MODE is set to LENGth.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:ACQuisition:SEConds <value>
[SENSE]:ACQuisition:SEConds?

Arguments <value>::=<NRf> specifies the acquisition length.

Examples SENSE:ACQUISITION:SAMPLES 12.5ms sets the acquisition length to 12.5 ms.

[SENSE]:{AM|FM|PM}:{BANDwidth|BWIDth}:MEASurement

Sets measurement bandwidth for the AM, FM, or PM demodulation to analyze.

Conditions	Measurement views: AM, FM, PM
Group	Sense commands
Syntax	<code>[SENSE]:{AM FM PM}:{BANDwidth BWIDth}:MEASurement <value></code> <code>[SENSE]:{AM FM PM}:{BANDwidth BWIDth}:MEASurement?</code>
Related Commands	FETCh:{AM FM PM}? READ:AM:RESult? READ:FM:RESult? READ:PM:RESult?
Arguments	<code><value>::=<Nrf></code> specifies the demodulation bandwidth for the specified modulation type.
Examples	<code>SENSE:AM:BANDwidth:MEASurement 1e6</code> sets the amplitude demodulation bandwidth to 1 MHz.

[SENSE]:{AM|FM|PM}:CLEar:RESults (No Query Form)

Clear results in the AM/FM/PM measurement.

Conditions	Measurement views: AM, FM, PM
Group	Sense commands
Syntax	<code>[SENSE]:{AM FM PM}:CLEar:RESults</code>
Arguments	None
Examples	<code>SENSE:AM:CLEAR:RESULTS</code> clears results in the AM measurement.

[SENSe]:{AM|FM|PM}:{MTPoints|MAXTracepoints}

Sets or queries the maximum trace points in the AM/FM/PM measurement.

Conditions	Measurement views: AM, FM, PM
Group	Sense commands
Syntax	[SENSe]:{AM FM PM}:{MTPoints MAXTracepoints} { ONEK TENK HUNDredk NDECimate NEVerdecimate } [SENSe]:{AM FM PM}:{MTPoints MAXTracepoints}?

Arguments The following table lists the arguments.

Argument	Maximum trace points
ONEK	1k
TENK	10k
HUNDredk	100k
NDECimate or NEVerdecimate	Never decimate

Examples SENSE:AM:MTPOINTS ONEK selects the maximum trace points of 1000 in the AM measurement.

[SENSe]:AM:DETECT:AMPLitude

Sets or queries the carrier amplitude detection method used to determine the 0% reference modulation in the AM measurement.

Conditions	Measurement views: AM
Group	Sense commands
Syntax	[SENSe]:AM:DETECT:AMPLitude { AVERAGE MEDIAN } [SENSe]:AM:DETECT:AMPLitude?
Arguments	AVERAGE defines the 0% reference modulation as the average amplitude in the analysis range (default). MEDIAN defines the 0% reference modulation as the median amplitude $([(\text{maximum})+(\text{minimum})]/2)$ in the analysis range.

Examples `SENSE:AM:DETECT:AMPLITUDE AVERAGE` defines the 0% modulation as the average amplitude in the analysis range.

[SENSe]:ANALysis:ADVanced:DITHer

Determines whether to enable or disable dithering, or set it automatically.

Dither is a random low-level signal consisting of white noise of one quantizing level peak-to-peak amplitude which may be added to an analog signal prior to sampling for the purpose of minimizing quantization error.

Conditions Measurement views: All

Group Sense commands

Syntax `[SENSe]:ANALysis:ADVanced:DITHer { AUTO | ON | OFF }`
`[SENSe]:ANALysis:ADVanced:DITHer?`

Arguments AUTO specifies that the dither is set automatically.
 ON enables dithering.
 OFF disables dithering.

Examples `SENSE:ANALYSIS:ADVANCED:DITHER ON` enables dithering.

[SENSe]:ANALysis:ADVanced:DITHer:HWARe:STATus? (Query Only)

Queries the dithering hardware status.

Conditions Measurement views: All

Group Sense commands

Syntax `[SENSe]:ANALysis:ADVanced:DITHer:HWARe:STATus?`

Arguments None

Returns One of the following status information.

Table 2-36: Dithering status

Status	Description
DUNaligned	Dithering is disabled and unaligned.
ON	Dithering is enabled
OFF	Dithering is disabled.

Examples `SENSE:ANALYSIS:ADVANCED:DITHER:HWARE:STATUS?` might return OFF, indicating that the dithering is disabled.

[SENSe]:ANALySis:LENGth

Sets or queries the analysis length. Programming a specified length sets [SENSe]:ANALySis:AUTO OFF.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:ANALySis:LENGth <value>
[SENSe]:ANALySis:LENGth?

Related Commands [\[SENSe\]:ANALySis:LENGth:AUTO](#)

Arguments <value> ::= <NRf> specifies the analysis length.
Range: 10 ns to [(acquisition length) - 400 ns].
If [(analysis start) + (analysis length)] > [(acquisition length) - 400 ns], the actual analysis length is reduced to [(acquisition length) - 200 ns].

Examples `SENSE:ANALYSIS:LENGTH 25.625us` sets the analysis length to 25.625 μ s.

[SENSe]:ANALySis:LENGth:ACTual? (Query Only)

Queries the actual analysis length.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:ANALysis:LENGth:ACTua1?

Arguments None

Returns <NRF> Actual analysis length in seconds.

Examples SENSE:ANALYSIS:LENGTH:ACTUAL? might return 25.625E-6, indicating that the actual analysis length is 25.625 μ s.

[SENSe]:ANALysis:LENGth:AUTO

Determines whether to set the analysis length automatically or manually.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:ANALysis:LENGth:AUTO { OFF | ON | 0 | 1 }
[SENSe]:ANALysis:LENGth:AUTO?

Arguments OFF or 0 sets the analysis length manually, using the [\[SENSe\]:ANALysis:LENGth](#) command.

ON or 1 sets the analysis length automatically.

Examples SENSE:ANALYSIS:LENGTH:AUTO ON sets the analysis length automatically.

[SENSe]:ANALysis:REFerence

Sets or queries the analysis time reference.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:ANALysis:REFerence { ACQSTART | TRIGGER }
[SENSe]:ANALysis:REFerence?

- Arguments** ACQSTART specifies the acquisition start as the time zero reference.
TRIGGER specifies the trigger point as the time zero reference.
- Examples** SENSE:ANALYSIS:REFERENCE ACQSTART specifies the acquisition start as the analysis time reference.

[SENSe]:ANALysis:START

Sets or queries the analysis offset time. Programming a specified offset time sets [SENSe]:ANALysis:START:AUTO OFF.

- Conditions** Measurement views: All
- Group** Sense commands
- Syntax** [SENSe]:ANALysis:START <value>
[SENSe]:ANALysis:START?
- Related Commands** [SENSe]:ANALysis:LENGth, [SENSe]:ANALysis:START:AUTO
- Arguments** <value>::=<NRF> specifies the analysis offset time.
Range: 0 to [(acquisition length) - 200 ns].
If [(analysis start) + (analysis length)] > [(acquisition length) - 400 ns], the actual analysis length is reduced to [(acquisition length) - 200 ns].
- Examples** SENSE:ANALYSIS:START 23.5us sets the analysis offset to 23.5 μ s.

[SENSe]:ANALysis:START:AUTO

Determines whether to set the analysis offset automatically or manually.

- Conditions** Measurement views: All
- Group** Sense commands
- Syntax** [SENSe]:ANALysis:START:AUTO { OFF | ON | 0 | 1 }
[SENSe]:ANALysis:START:AUTO?

- Arguments** OFF or 0 sets the analysis offset manually, using the [\[SENSe\]:ANALysis:START](#) command.
ON or 1 sets the analysis offset automatically.
- Examples** `SENSE:ANALYSIS:START:AUTO ON` sets the analysis offset automatically.

[SENSe]:AVTime:{BANDwidth|BWIDth}

Sets or queries the time-domain bandwidth filter in the Amplitude versus Time measurement. Programming a specified bandwidth disables the [\[SENSe\]:AVTime:SPAN](#) setting.

- Conditions** Measurement views: Amplitude versus Time
- Group** Sense commands
- Syntax** `[SENSe]:AVTime:{BANDwidth|BWIDth} <value>`
`[SENSe]:AVTime:{BANDwidth|BWIDth}?`
- Arguments** `<value>::=<NRF>` specifies the filter bandwidth.
Range: 1 Hz to 20 MHz (Standard) / 60 MHz (Option 110).
- Examples** `SENSE:AVTIME:BANDWIDTH 10MHZ` sets the filter bandwidth to 10 MHz.

[SENSe]:AVTime:{BANDwidth|BWIDth}:ACTual? (Query Only)

Queries the actual time-domain bandwidth in the Amplitude versus Time measurement.

- Conditions** Measurement views: Amplitude versus Time
- Group** Sense commands
- Syntax** `[SENSe]:AVTime:{BANDwidth|BWIDth}:ACTual?`
- Arguments** None

Returns <NRf> The actual time-domain bandwidth in Hz.

Examples SENSE:AVTIME:BANDWIDTH:ACTUAL? might return 20E+6, indicating that the actual time-domain bandwidth is 20 MHz.

[SENSE]:AVTime:CLEAr:RESuLts (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Conditions Measurement views: Amplitude versus Time

Group Sense commands

Syntax [SENSE]:AVTime:CLEAr:RESuLts

Arguments None

Examples SENSE:AVTIME:CLEAR:RESULTS restarts multi-trace functions.

[SENSE]:AVTime:MAXTracepoints

Sets or queries the maximum trace points in the Amplitude versus Time measurement.

Conditions Measurement views: Amplitude versus Time

Group Sense commands

Syntax [SENSE]:AVTime:MAXTracepoints { ONEK | TENK | HUNDredk | NEVERdecimate }
[SENSE]:AVTime:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
TENK sets the maximum trace points to 10 k.
HUNDredk sets the maximum trace points to 100 k.
NEVERdecimate never decimates the trace points.

Examples `SENSE:AVTIME:MAXTRACEPOINTS TENK` sets the maximum trace points to 10 k.

[SENSe]:AVTime:METhod

Sets or queries the method to set the measurement bandwidth in the Amplitude versus Time measurement.

Conditions Measurement views: Amplitude versus Time

Group Sense commands

Syntax `[SENSe]:AVTime:METhod { SPAN | TDBW }`
`[SENSe]:AVTime:METhod?`

Arguments `SPAN` specifies that the measurement bandwidth is set by the frequency span, using the `[SENSe]:AVTime:SPAN` command.

`TDBW` specifies that the measurement bandwidth is set by the time-domain bandwidth, using the `[SENSe]:AVTime:{BANDwidth|BWIDth}` command.

Examples `SENSE:AVTIME:METHOD SPAN` specifies that the measurement bandwidth is set by the frequency span.

[SENSe]:AVTime:SPAN

Sets or queries the frequency span in the Amplitude versus Time measurement. Programming a specified span disables the `[SENSe]:AVTime:{BANDwidth|BWIDth}` setting.

Conditions Measurement views: Amplitude versus Time

Group Sense commands

Syntax `[SENSe]:AVTime:SPAN <value>`
`[SENSe]:AVTime:SPAN?`

Arguments `<value>::=<Nrf>` specifies the frequency span.
Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)

Examples `SENSE:AVTIME:SPAN 5MHZ` sets the frequency span to 5 MHz.

[SENSe]:CCDF:{BANDwidth|BWIDth}

Sets or queries the CCDF measurement bandwidth (frequency span).

Conditions Measurement views: CCDF

Group Sense commands

Syntax `[SENSe]:CCDF:{BANDwidth|BWIDth} <value>`
`[SENSe]:CCDF:{BANDwidth|BWIDth}?`

Arguments `<value> ::= <NRf>` is the CCDF measurement bandwidth.
 Range: 10 Hz to 40 MHz (Standard) / 60 MHz (Option 110).

Examples `SENSE:CCDF:BANDWIDTH 1MHZ` sets the CCDF measurement bandwidth to 1 MHz.

[SENSe]:CCDF:CLEAr (No Query Form)

Clears the CCDF accumulator and restarts the measurement.

Conditions Measurement views: CCDF

Group Sense commands

Syntax `[SENSe]:CCDF:CLEAr`

Arguments None

Examples `SENSE:CCDF:CLEAr` clears the CCDF accumulator and restarts the measurement.

[SENSe]:CCDF:TIME:TOTAl:LENGth

Sets or queries the CCDF measurement time when `[SENSe]:CCDF:TIME:TYPE` is set to `TOTAl`.

Conditions	Measurement views: CCDF
Group	Sense commands
Syntax	[SENSe]:CCDF:TIME:TOTAl:LENGth <value> [SENSe]:CCDF:TIME:TOTAl:LENGth?
Arguments	<value> ::= <NRf> specifies the CCDF measurement time. Range: 20 ms to 100 s.
Examples	SENSe:CCDF:TIME:TOTAl:LENGth 10 sets the CCDF measurement time to 10 s.

[SENSe]:CCDF:TIME:TYPE

Determines how to repeat the CCDF measurement.

Conditions	Measurement views: CCDF
Group	Sense commands
Syntax	[SENSe]:CCDF:TIME:TYPE { SINGLE TOTAl CONTInuous } [SENSe]:CCDF:TIME:TYPE?
Related Commands	INITiate commands
Arguments	<p>SINGLE specifies that the analyzer sets the analysis length to 1 ms and then acquire data once to calculate CCDF.</p> <p>TOTAl specifies that the analyzer sets the analysis length to 20 ms and then repeats data acquisition and CCDF calculation for the time specified by the [SENSe]:CCDF:TIME:TOTAl:LENGth command.</p> <p>CONTInuous specifies that the analyzer sets the analysis length to 1 ms and then repeats data acquisition and CCDF calculation continuously. To reset the process, use the [SENSe]:CCDF:CLEAr command or the INITiate commands.</p>
Examples	SENSe:CCDF:TIME:TYPE SINGLE specifies that the analyzer sets the analysis length to 1 ms and then acquire data once to calculate CCDF.

[SENSe]:DDEMod:ANALysis:LENGth

Sets or queries the analysis length in seconds or symbols. The command [\[SENSe\]:DDEMod:TIME:UNITs](#) determines which is used. For example, if the symbol rate is 1 MHz and the acquisition length is 20 ms, the range may be 0 to 19999. Setting a specified length changes [\[SENSe\]:DDEMod:ANALysis:AUTO](#) to OFF.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [\[SENSe\]:DDEMod:ANALysis:LENGth <value>](#)
[\[SENSe\]:DDEMod:ANALysis:LENGth?](#)

Related Commands [\[SENSe\]:DDEMod:ANALysis:LENGth:ACTual?](#)
[\[SENSe\]:DDEMod:TIME:UNITs](#)
[\[SENSe\]:DDEMod:ANALysis:LENGth:AUTO](#)

Arguments `<value> ::= <NRF>` specifies the analysis length in seconds or symbols.
 Range in seconds: 200 ns to [(acquisition length) - 400 ns].
 If [(analysis start) + (analysis length)] > [(acquisition length) - 400 ns], the actual analysis length is reduced to [(acquisition length) - 200 ns].
 Range in symbols: 200 ns * (symbol rate) to [(acquisition length) - 400 ns] * (symbol rate).
 If [(analysis start) + (analysis length)] > [(acquisition length) - 400 ns], the actual analysis length is reduced to [(acquisition length) - 200 ns] * (symbol rate).

Examples `SENSE:DDEMOD:ANALYSIS:LENGTH 25.625us` sets the analysis length to 25.625 μ s.
`SENSE:DDEMOD:ANALYSIS:LENGTH 256` sets the analysis length to 256 symbols.

[SENSe]:DDEMod:ANALysis:LENGth:ACTual? (Query Only)

Queries the actual analysis length which returns a value in either seconds or symbols. The command [\[SENSe\]:DDEMod:TIME:UNITs](#) determines which is used.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands
Syntax	[SENSe]:DDEMod:ANALysis:LENGth:ACTual?
Related Commands	[SENSe]:DDEMod:ANALysis:LENGth [SENSe]:DDEMod:TIME:UNITs
Arguments	None
Returns	<NRF> Actual analysis length in seconds or symbols.
Examples	SENSE:DDEMOD:ANALYSIS:LENGTH:ACTUAL? might return 25.625E-6, indicating that the actual analysis length is 25.625 μs.

[SENSe]:DDEMod:ANALysis:LENGth:AUTO

Determines whether to set the analysis length automatically or manually.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands
Syntax	[SENSe]:DDEMod:ANALysis:LENGth:AUTO { OFF ON 0 1 } [SENSe]:DDEMod:ANALysis:LENGth:AUTO?
Arguments	OFF or 0 sets the analysis length manually, using the [SENSe]:DDEMod:ANALysis:LENGth command. ON or 1 sets the analysis length automatically.
Examples	SENSE:DDEMOD:ANALYSIS:LENGTH:AUTO ON sets the analysis length automatically.

[SENSe]:DDEMod:{BANDwidth|BWIDth}:MODE

Sets or queries the measurement bandwidth mode for Digital Demod measurements.

Conditions Measurement views: General purpose digital modulation

Group Sense group

Syntax [SENSe]:DDEMod:{BANDwidth|BWIDth}:MODE { MANua1 | AUTO | LSPan }
[SENSe]:DDEMod:{BANDwidth|BWIDth}:MODE?

Related Commands [\[SENSe\]:DDEMod:{BANDwidth|BWIDth}:TINTerval](#)

Arguments MANua1 specifies manual bandwidth control mode. A typical use is setting a narrow measurement bandwidth on a small range of frequencies to examine one signal while rejecting the others that are present in a Spectrum graph.

AUTO specifies automatic bandwidth control mode where a measurement picks a bandwidth based on other parameter settings (such as symbol rate, modulation type, filter, and so on).

LSPan (LinkToSpan) specifies Lspan bandwidth control mode, where you can use the Spectrum display to tune the frequency, view the signal, and use the Span control to set the measurement bandwidth. This mode emulates legacy instruments.

Examples DDEMOD:BANDWIDTH:MODE AUTO sets the analyzer bandwidth mode to automatically select a measurement bandwidth.

[SENSe]:DDEMod:{BANDwidth|BWIDth}:TINTerval

Sets or queries the measurement bandwidth (frequency span).

Conditions Measurement views: General purpose digital modulation

Group Sense group

Syntax [SENSe]:DDEMod:{BANDwidth|BWIDth}:TINTerval <value>
[SENSe]:DDEMod:{BANDwidth|BWIDth}:TINTerval?

Related Commands [\[SENSe\]:DDEMod:SRATe](#)

Arguments <value> ::= <NRF> specifies the measurement bandwidth.
 Range: Symbol rate to 40 MHz or, with Option 110, 110 MHz.
 The minimum value depends on the setting of [:SENSe]:DDEMod:SRATe.

Returns <NRF> Actual measurement bandwidth.

Examples SENSE:DDEMOD:BANDWIDTH:TINTERVAL 35.255MHZ sets the measurement bandwidth to 35.255 MHz.

[SENSe]:DDEMod:{BANDwidth|BWIDth}:TINTerval:AUTO

Sets or queries the measurement bandwidth (frequency span) automatically.

Conditions Measurement views: General purpose digital modulation

Group Sense group

Syntax [SENSe]:DDEMod:{BANDwidth|BWIDth}:TINTerval:AUTO { OFF | ON
 | 0 | 1 }
 [SENSe]:DDEMod:{BANDwidth|BWIDth}:TINTerval:AUTO?

Related Commands [\[SENSe\]:DDEMod:{BANDwidth|BWIDth}:TINTerval](#)

Arguments OFF or 0 sets the measurement bandwidth manually, using the [\[SENSe\]:DDEMod:{BANDwidth|BWIDth}:TINTerval](#) command.
 ON or 1 sets the measurement bandwidth automatically.

Examples SENSE:DDEMOD:BANDWIDTH:TINTERVAL:AUTO sets the measurement bandwidth automatically.

[SENSe]:DDEMod:BURSt:DETect

Sets or queries burst detection.

Conditions Measurement views: General purpose digital modulation

Group	Sense commands
Syntax	[SENSE]:DDEMod:BURSt:DETECT { ON OFF } [SENSE]:DDEMod:BURSt:DETECT?
Related Commands	[SENSe]:DDEMod:BURSt:THReshold
Arguments	ON analyzes just that burst period if a burst is found. If a burst is not found, does not analyze but displays an error message. OFF analyzes the whole analysis length. <hr/> <i>NOTE. When selecting On and if the signal is not adequate for the demodulation, the measurement will fail and show an error message.</i> <hr/>
Examples	SENSE:DDEMOD:BURST:DETECT OFF disables burst detection and analyzes the whole analysis length.

[SENSe]:DDEMod:BURSt:THReshold

Sets or queries the threshold level above which the input signal is determined to be a burst.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands
Syntax	[SENSe]:DDEMod:BURSt:THReshold <value> [SENSe]:DDEMod:BURSt:THReshold?
Related Commands	[SENSe]:DDEMod:BURSt:DETECT
Arguments	<value> ::= <NRf> specifies the threshold level for detecting bursts. Range: -100 to -10 dBc.
Examples	SENSE:DDEMOD:BURST:THRESHOLD -25 sets the threshold level to -25 dBc.

[SENSe]:DDEMod:CARRier:OFFSet

Sets or queries the carrier frequency offset in digital modulation analysis.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands
Syntax	[SENSe]:DDEMod:CARRier:OFFSet <value> [SENSe]:DDEMod:CARRier:OFFSet?
Related Commands	The settings of the following commands may narrow the effective range. [SENSe]:DDEMod:FILTer:ALPHa [SENSe]:DDEMod:FILTer:REFerence [SENSe]:DDEMod:MODulation:TYPE [SENSe]:DDEMod:SRATe
Arguments	<value> ::= <Nrf> specifies the carrier frequency offset. Range: -20 MHz to +20 MHz or with Option 110, -55 MHz to +55 MHz .
Examples	SENSE:DDEMOD:CARRIER:OFFSET 2kHz sets the carrier frequency offset to 2 kHz.

[SENSe]:DDEMod:CARRier:OFFSet:AUTO

Sets or queries whether to detect the carrier frequency automatically in digital modulation analysis.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands
Syntax	[SENSe]:DDEMod:CARRier:OFFSet:AUTO { OFF ON 0 1 } [SENSe]:DDEMod:CARRier:OFFSet:AUTO?
Related Commands	[SENSe]:DDEMod:CARRier:OFFSet

- Arguments** OFF or 0 sets the carrier frequency manually, using the `[SENSE]:DDEMod:CARRier:OFFSet` command.
- ON or 1 detects the carrier frequency automatically.
- Examples** `[SENSE]:DDEMOD:CARRIER:OFFSET:AUTO ON` enables automatic detection of the carrier frequency.

[SENSE]:DDEMod:FILTer:ALPHa

Sets or queries the filter factor (α/BT) in the digital modulation analysis.

- Conditions** Measurement views: General purpose digital modulation
- Group** Sense commands
- Syntax** `[SENSE]:DDEMod:FILTer:ALPHa <value>`
`[SENSE]:DDEMod:FILTer:ALPHa?`
- Arguments** `<value>::=<Nrf>` specifies the filter factor. Range: 0.001 to 1.
- Examples** `SENSE:DDEMOD:FILTER:ALPHA 0.5` sets the filter factor to 0.5.

[SENSE]:DDEMod:FILTer:MEASurement

Sets or queries the measurement filter in the digital modulation analysis.

- Conditions** Measurement views: General purpose digital modulation
- Group** Sense commands
- Syntax** `[SENSE]:DDEMod:FILTer:MEASurement { OFF | RRCosine | RCOSine | GAUSSian | RECTangular | IS95TXEQ_MEA | IS95TX_MEA | C4FM_P25 | USERx | UOTHer }`
`[SENSE]:DDEMod:FILTer:MEASurement?`

Arguments The following table lists the arguments.

Table 2-37: Digital modulation measurement filter

Argument	Measurement filter
OFF	No filter
RRCosine	Root Raised Cosine
RCOSine	Raised Cosine
GAUSSian	Gaussian
RECTangular	Rectangular
IS95TXEQ_MEA	IS95 receive filter for the transmitter configured with both the transmit filter and the phase equalizer.
IS95TX_MEA	IS95 receive filter for the transmitter configured with only the transmit filter.
C4FM_P25	C4FM-P25
USER1	User defined Measurement Filter 1
USER2	User defined Measurement Filter 2
USER3	User defined Measurement Filter 3
UOTHer	Other user defined Measurement Filter

Examples `SENSE:DDEMOD:FILTER:MEASUREMENT RRCosine` selects the Root Raised Cosine filter as the measurement filter.

[SENSE]:DDEMod:FILTER:REFERENCE

Sets or queries the reference filter in the digital modulation analysis.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax `[SENSE]:DDEMod:FILTER:REFERENCE { OFF | RCOSine | GAUSSian | RECTangular | IS95REF | HSINE | SOQPSK_MIL | SOQPSK_ARTM | SBPSK_MIL | USERx | UOTHer }`
`[SENSE]:DDEMod:FILTER:REFERENCE?`

Arguments The following table lists the arguments.

Table 2-38: Digital modulation reference filter

Argument	Measurement filter
OFF	No filter
RCOSine	Raised Cosine
GAUSSian	Gaussian
RECTangular	Rectangular
IS95REF	IS95 reference filter including the response of the transmit filter, the phase equalizer, and the receive (complementary) filter.
HSINe	Half Sine
SOQPSK_MIL	SOQPSK-MIL
SOQPSK_ARTM	SOQPSK-ARTM
SBPSK_MIL	SBPSK-MIL
USER1	User defined Measurement Filter 1
USER2	User defined Measurement Filter 2
USER3	User defined Measurement Filter 3
UOTHer	Other user defined Measurement Filter

Examples `SENSE:DDEMOD:FILTER:REFERENCE RCOSine` selects the Raised Cosine filter as the reference filter.

[SENSe]:DDEMod:FREQuency:DEVIation

Sets or queries the frequency deviation in the digital modulation analysis. Programming a specified frequency deviation sets `[SENSe]:DDEMod:FREQuency:DEVIation:AUTO OFF`.

This command is valid when `[SENSe]:DDEMod:MODulation:TYPE` is set to C4FM, FSK2, FSK4, FSK8, or FSK16.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax `[SENSe]:DDEMod:FREQuency:DEVIation <value>`
`[SENSe]:DDEMod:FREQuency:DEVIation?`

- Arguments** <value>::=<Nrf> sets the frequency deviation.
 Standard product range: 1 Hz to 40 MHz.
 Option 110 product range: 1 Hz to 110 MHz.
- Examples** SENSE:DDEMOD:FREQUENCY:DEVIATION 1MHZ sets the frequency deviation to 1 MHz.

[SENSe]:DDEMod:FREQuency:DEVIation:AUTO

Determines whether to detect automatically or set manually the frequency deviation used to determine the symbol values of an FSK or C4FM signal.

This command is valid when [SENSe]:DDEMod:MODulation:TYPE is set to C4FM, FSK2, FSK4, FSK8, or FSK16.

- Conditions** Measurement views: General purpose digital modulation
- Group** Sense commands
- Syntax** [SENSe]:DDEMod:FREQuency:DEVIation:AUTO { OFF | ON | 0 | 1 }
 [SENSe]:DDEMod:FREQuency:DEVIation:AUTO?
- Arguments** ON or 1 automatically calculates the frequency deviation for the analysis range (default).
 OFF or 0 sets the frequency deviation using the [SENSe]:DDEMod:FREQuency:DEVIation command.
- Examples** SENSE:DDEMOD:FREQUENCY:DEVIATION:AUTO ON automatically calculates the frequency deviation.

[SENSe]:DDEMod:MAGNitude:NORMALize

Sets or queries the method for the magnitude normalization.

- Conditions** Measurement views: General purpose digital modulation
- Group** Sense commands

Syntax [SENSe]:DDEMod:MAGNitude:NORMALize { RSYMBOL | MSYMBOL }
[SENSe]:DDEMod:MAGNitude:NORMALize?

Arguments RSYMBOL normalizes the magnitude with the RMS symbol magnitude.
MSYMBOL normalizes the magnitude with the maximum symbol magnitude.

Examples SENSE:DDEMOD:MAGNITUDE:NORMALIZE RSYMBOL normalizes the magnitude with the RMS symbol magnitude.

[SENSe]:DDEMod:MINDEX

Sets or queries the modulation index of a CPM signal. This command is valid when [SENSe]:DDEMod:MODulation:TYPE is set to CPM and [SENSe]:DDEMod:MINDEX:AUTO is set to OFF.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [SENSe]:DDEMod:MINDEX { 1 | 2 | 3 | 4 | 5 | 6 }
[SENSe]:DDEMod:MINDEX?

Arguments The following table shows the arguments and modulation index.

CPM modulation index

Argument	Modulation index
1	4/16, 5/16
2	5/16, 6/16
3	6/16, 7/16
4	7/16, 10/16
5	12/16, 13/16
6	8/16, 8/16

Examples SENSE:DDEMOD:MINDEX 1 selects the modulation index to “4/16, 5/16”.

[SENSe]:DDEMod:MINdex:AUTO

Determines whether to detect automatically or set manually the modulation index of a CPM signal. This command is valid when [SENSe]:DDEMod:MODulation:TYPE is set to CPM.

- Conditions** Measurement views: General purpose digital modulation

- Group** Sense commands

- Syntax** [SENSe]:DDEMod:MINdex:AUTO { OFF | ON | 0 | 1 }
[SENSe]:DDEMod:MINdex:AUTO

- Arguments** ON or 1 automatically calculates the modulation index for the analysis range.

OFF or 0 sets the modulation index using the [SENSe]:DDEMod:MINdex command.

- Examples** SENSE:DDEMOD:MINDEX:AUTO ON automatically calculates the modulation index for the analysis range.

[SENSe]:DDEMod:MODulation:TYPE

Sets or queries the modulation type in the digital modulation analysis.

- Conditions** Measurement views: General purpose digital modulation

- Group** Sense commands

- Syntax** [SENSe]:DDEMod:MODulation:TYPE { QPSK | PSK8 | D8PSK |
PIOVER2DBPSK | DQPSK | PIOVER4DQPSK | BPSK | OQPSK | QAM16 |
QAM32 | QAM64 | QAM128 | QAM256 | MSK | FSK2 | FSK4 | FSK8
| FSK16 | CPM | SOQPSK | SBPSK | C4FM }
[SENSe]:DDEMod:MODulation:TYPE?

- Arguments** The following table lists the arguments and corresponding modulation type.

Table 2-39: Modulation type

Argument	Modulation type
QPSK	QPSK

Table 2-39: Modulation type (cont.)

Argument	Modulation type
PSK8	8PSK
D8PSK	D8PSK
PIOVER2DBPSK	$\pi/2$ DBPSK
DQPSK	DQPSK
PIOVER4DQPSK	$\pi/4$ QPSK
BPSK	BPSK
OQPSK	OQPSK
QAM16	16QAM
QAM32	32QAM
QAM64	64QAM
QAM128	128QAM
QAM256	256QAM
MSK	MSK
FSK2	FSK2
FSK4	FSK4
FSK8	FSK8
FSK16	FSK16
CPM	CPM
SOQPSK	SOQPSK
SBPSK	SBPSK
C4FM	C4FM

Examples `SENSE:DDEMOD:MODULATION:TYPE QPSK` selects QPSK modulation system.

[SENSe]:DDEMod:PRESet (No Query Form)

Presets the modulation analysis to a communication standard.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax `[SENSe]:DDEMod:PRESet <standard_name>`

Related Commands [\[SENSe\]:DDEMod:MODulation:TYPE](#)

Arguments The following table lists the preset standard names with their modulation types and settings.

Table 2-40: Modulation Presets

Preset Name	Modulation type	Settings
"802.15.4"	OQPSK	Symbol rate: 1 MHz Meas Filter: None Ref Filter: Half sine Filter Param: None Symbol Pt Location: NA Remove Q offset: not checked
"SBPSK-MIL"	SBPSK	Symbol rate: 2.4 kHz Meas Filter: None Ref Filter: SBPSK-MIL Filter Param: 0.5 Symbol Pt Location: NA Remove Q offset: NA
"SOQPSK-MIL"	SOQPSK	Symbol rate: 2.4 kHz Meas Filter: None Ref Filter: SOQPSK-MIL Filter Param: 0.5 Symbol Pt Location: Center Remove Q offset: checked
"CPM-MIL"	CPM	Symbol rate: 19.2 KHz Meas Filter: None Ref Filter: None Filter Param: None Symbol Pt Location: NA Remove Q offset: NA
"SOQPSK-ARTM Tier 1"	SOQPSK	Symbol rate: 2.5 MHz Meas Filter: None Ref Filter: SOQPSK-ARTM Filter Param: None Symbol Pt Location: Center Remove Q offset: checked

Table 2-40: Modulation Presets (cont.)

Preset Name	Modulation type	Settings
"Project25 Phase I"	C4FM	Symbol rate: 4.8 kHz
		Meas Filter: C4FM-P25
		Ref Filter: Raised cosine
		Filter Param: 0.2
		Symbol Pt Location: NA
		Remove Q offset: NA
"CDMA2000-Base"	QPSK	Symbol rate: 1.2288 MHz
		Meas Filter: IS95 TXEQ_MEA
		Ref Filter: IS95 REF
		Filter Param: None
		Symbol Pt Location: NA
		Remove Q offset: NA
"W-CDMA"	QPSK	Symbol rate: 3.84 MHz
		Meas Filter: Root raised cosine
		Ref Filter: Raised cosine
		Filter Param: 0.22
		Symbol Pt Location: NA
		Remove Q offset: NA

In addition to the specific settings listed in the table, the following general settings are also made when you load any of the defined presets.

Setting	Value
Points/symbol	4
Burst detection mode	Off
Burst detection threshold	-10 dBc
Analysis offset	Auto
Analysis length	Auto
Frequency offset	Auto
Measurement BW	Auto
Frequency deviation	Auto
Modulation index	Auto

Returns

Examples [SENSE]:DDEMOD:PRESET "802.15.4" sets demodulation to the standard OQPSK modulation.

[SENSe]:DDEMod:SRATe

Sets or queries the symbol rate in the digital modulation analysis.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [SENSe]:DDEMod:SRATe <value>
[SENSe]:DDEMod:SRATe?

Arguments <value>::=<NRF> specifies the symbol rate.
Standard product range: 100 Hz to 40 MHz.
Option 110 product range: 100 Hz to 110 MHz.

Examples SENSE:DDEMOD:SRATE 21.0E3 sets the symbol rate to 21 kHz.

[SENSe]:DDEMod:SWAP:IQ

Determines whether or not to exchange I and Q data before demodulating.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [SENSe]:DDEMod:SWAP:IQ { OFF | ON | 0 | 1 }
[SENSe]:DDEMod:SWAP:IQ?

Arguments OFF or 0 uses I and Q data as they are.
ON or 1 exchanges I and Q data.

Examples SENSE:DDEMOD:SWAP:IQ ON exchanges I and Q data before demodulating.

[SENSe]:DDEMod:SYMBol:HSSHift

Sets or queries the Q data half-symbol shift for OQPSK and SOQPSK signals.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands
Syntax	[SENSe]:DDEMod:SYMBOL:HSSHift { OFF ON 0 1 } [SENSe]:DDEMod:SYMBOL:HSSHift?
Related Commands	[SENSe]:DDEMod:MODulation:TYPE
Arguments	OFF or 0 the Q offset shift is not applied. ON or 1 the Q offset shift is applied.
Examples	DDEMod:SYMBOL:HSSHift ON the Q offset is applied.

[SENSe]:DDEMod:SYMBOL:MAP:SOURce? (Query Only)

Queries the user symbol map.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands
Syntax	[SENSe]:DDEMod:SYMBOL:MAP:SOURce?
Arguments	None.
Examples	SENSE:DDEMOD:SYMBOL:MAP:SOURCE? returns the symbol map filename.

[SENSe]:DDEMod:SYMBOL:MAP[:STATe]

Determines whether or not to use the user symbol map.

Conditions	Measurement views: General purpose digital modulation
Group	Sense commands

Syntax [SENSE]:DDEMod:SYMBOL:MAP[:STATE] { OFF | ON | 0 | 1 }
[SENSE]:DDEMod:SYMBOL:MAP[:STATE]?

Related Commands [SENSE]:DDEMod:SYMBOL:MAP:SOURce?

Arguments OFF or 0 disables the user symbol map.
ON or 1 enables the user symbol map.

Examples SENSE:DDEMOD:SYMBOL:MAP:STATE ON enables the user symbol map.

[SENSE]:DDEMod:SYMBOL:PLOT:POSITION

Sets or queries the symbol point location on an SOQPSK waveform.

Conditions Effective only on an SOQPSK waveform and on any general purpose digital demodulation views except Signal Quality and Symbol Table.

Group Sense commands

Syntax [SENSE]:DDEMod:SYMBOL:PLOT:POSITION { EDGE | MIDDLE }
[SENSE]:DDEMod:SYMBOL:PLOT:POSITION?

Related Commands

Arguments EDGE sets the symbol location at the edge of the eye opening.
MIDDLE sets the symbol location at the middle of the eye opening.

Examples [SENSE]:DDEMOD:SYMBOL:PLOT:POSITION EDGE sets the symbol location the edge of the eye opening.

[SENSE]:DDEMod:SYMBOL:POINTS

Sets or queries the number of points per symbol (how many points to use between symbols when connecting the dots).

NOTE. 1 is not valid for the GMSK modulation.

In the constellation view, select VECTors using the TRACe:CONSt:MODE command first to change Points/Symbol.

Conditions Measurement views: Constellation, EVM versus Time, Magnitude error versus Time, Phase error versus Time, Freq Dev versus Time, Demod I&Q versus Time.

Group Sense commands

Syntax [SENSE]:DDEMod:SYMBOL:POINTS { ONE | TWO | FOUR | EIGHT }
[SENSE]:DDEMod:SYMBOL:POINTS?

Arguments ONE, TWO, FOUR, and EIGHT represent the number of points per symbol. The following table lists the conditions of use.

Argument	Modulation type supported
ONE	All but SOQPSK, OQPSK, SBPSK
TWO	All but SOQPSK
FOUR	All
EIGHT	All

Examples SENSE:DDEMOD:SYMBOL:POINTS FOUR sets the number of points per symbol to four.

[SENSE]:DDEMod:SYMBOL:RATE:SEARCH

Determines whether to enable a symbol rate search. This command is valid when the demodulation type is set to FSK2, FSK4, FSK8 or FSK16.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [SENSE]:DDEMod:SYMBOL:RATE:SEARCH { OFF | ON | 0 | 1 }

Related Commands [\[SENSE\]:DDEMod:MODulation:TYPE](#)

Arguments OFF or 0 disables the search.
ON or 1 enables the search.

Examples [SENSE]:DDEMOD:SYMBOL:RATE:SEARCH ON enables the symbol rate search.

[SENSe]:DDEMod:SYNCh:WORD

Determines whether to enable the synchronization word.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [SENSe]:DDEMod:SYNCh:WORD { OFF | ON | 0 | 1 }
[SENSe]:DDEMod:SYNCh:WORD?

Related Commands [\[SENSe\]:DDEMod:SYNCh:WORD:SYMBol](#)

Arguments OFF or 0 disables the synchronization word.
ON or 1 enables the synchronization word.

Examples SENSE:DDEMOD:SYNCH:WORD ON enables the synchronization word.

[SENSe]:DDEMod:SYNCh:WORD:SYMBol

Sets or queries the synchronization word when [\[SENSe\]:DDEMod:SYNCh:WORD](#) is ON. The word depends on the modulation type selected by the [\[SENSe\]:DDEMod:MODulation:TYPE](#) command.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [SENSe]:DDEMod:SYNCh:WORD:SYMBol <block>
[SENSe]:DDEMod:SYNCh:WORD:SYMBol?

Arguments <block>::=#<num_digit><num_byte><sym(1)><sym(2)>...<sym(n)>

Where
<num_digit> is the number of digits in <num_byte>.
<num_byte> is the number of bytes of data that follow.

<sym(n)> is the nth symbol value of the sync word. 32-bit integer.
n: Max 256.

Examples SENSE:DDEMOD:SYNCH:WORD:SYMBOL #216xxxx (4 symbols) sets a sync word composed of four symbols.

[SENSe]:DDEMod:TIME:UNITs

Sets or queries the fundamental unit of time.

Conditions Measurement views: General purpose digital modulation

Group Sense commands

Syntax [SENSe]:DDEMod:TIME:UNITs { SECONDS | SYMBOLs }
[SENSe]:DDEMod:TIME:UNITs?

Arguments SECONDS specifies the fundamental unit of time as seconds.
SYMBOLs specifies the fundamental unit of time as symbols.

Examples SENSE:DDEMOD:TIME:UNITs SECONDS specifies the fundamental unit of time as seconds.

[SENSe]:DPSA:AUDio:DEMod:GAIN

Sets or queries the audio gain.

NOTE. *The sound level is also affected by the Windows volume control.*

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax [SENSe]:DPSA:AUDio:DEMod:GAIN <value>
[SENSe]:DPSA:AUDio:DEMod:GAIN?

Arguments <value> ::= <NR1> specifies the audio gain. Range: 0 to 15 (integer).

Examples `SENSE:DPSA:AUDIO:DEMODO:GAIN 7` sets the audio gain to 7.

[SENSe]:DPSA:AUDio:DEMod:RXBWidth

Sets or queries the receiver bandwidth in the audio demodulation.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax `[SENSe]:DPSA:AUDio:DEMod:RXBwidth <value>`
`[SENSe]:DPSA:AUDio:DEMod:RXBwidth?`

Arguments `<value>::=<Nrf>` specifies the receiver bandwidth in the audio demodulation.
 Range: 1 kHz to 500 kHz.

Examples `SENSE:DPSA:AUDIO:DEMODO:RXBWIDTH 30kHz` sets the receiver bandwidth to 30 kHz.

[SENSe]:DPSA:AUDio:DEMod:RXFrequency? (Query Only)

Returns the receiver frequency in the audio demodulation. The frequency depends on the setting of the [\[SENSe\]:DPSA:AUDio:DEMod:TUNE](#) command.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax `[SENSe]:DPSA:AUDio:DEMod:RXFrequency?`

Arguments None

Returns `<frequency>::=<Nrf>` is the receiver frequency in the audio demodulation.

Examples `SENSE:DPSA:AUDIO:DEMODO:RXFREQUENCY?` might return `80.3E+6`, indicating that the receiver frequency is 80.3 MHz.

[SENSe]:DPSA:AUDio:DEMod:STATe

Determines whether to enable the audio demodulation.

Conditions	Measurement views: DPX spectrum
Group	Sense commands
Syntax	[SENSe]:DPSA:AUDio:DEMod:STATe { OFF ON 0 1 } [SENSe]:DPSA:AUDio:DEMod:STATe?
Arguments	OFF or 0 disables the audio demodulation. ON or 1 enables the audio demodulation.
Examples	SENSE:DPSA:AUDIO:DEMOD:STATE ON enables the audio demodulation.

[SENSe]:DPSA:AUDio:DEMod:TUNE

Sets or queries how to determine the tuning frequency in the audio demodulation.

Conditions	Measurement views: DPX spectrum
Group	Sense commands
Syntax	[SENSe]:DPSA:AUDio:DEMod:TUNE { MR MARK1 MARK2 MARK3 MARK4 SMARkeR FREQcontroL } [SENSe]:DPSA:AUDio:DEMod:TUNE?
Arguments	The following table lists the arguments.

Table 2-41: Frequency tuning

Argument	Tune with
MR	Reference marker (MR)
MARK1	Marker 1 (M1)
MARK2	Marker 2 (M2)
MARK3	Marker 3 (M3)
MARK4	Marker 4 (M4)

Table 2-41: Frequency tuning (cont.)

Argument	Tune with
SMARker	Selected marker
FREQcontrol	Center frequency setting

Examples `SENSE:DPSA:AUDIO:DEMOD:TUNE MARK1` sets the tuning frequency to the value at Marker 1.

[SENSe]:DPSA:AUDio:DEMod:TYPE

Sets or queries the modulation type in the audio demodulation.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax `[SENSe]:DPSA:AUDio:DEMod:TYPE { AM | FM }`
`[SENSe]:DPSA:AUDio:DEMod:TYPE?`

Arguments AM selects the AM (Amplitude Modulation).
 FM selects the FM (Frequency Modulation).

Examples `SENSE:DPSA:AUDIO:DEMOD:TYPE FM` selects FM in the audio demodulation.

[SENSe]:DPSA:{BANDwidth|BWIDth}:ACTual? (Query Only)

Queries the actual bandwidth whether set automatically or manually.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax `[SENSe]:DPSA:{BANDwidth|BWIDth}:ACTual?`

Related Commands [\[SENSe\]:DPSA:{BANDwidth|BWIDth}:OPTimization](#)

Arguments None

Examples `SENSE:DPSA:BANDWIDTH:ACTUAL?` returns the RBW as a percentage of the Span.

[SENSe]:DPSA:{BANDwidth|BWIDth}:OPTimization

Sets or queries the RF & IF Optimization for the Spectrum display and the Option 200 DPX Spectrum displays. The settings optimize the gain and bandwidth in the RF and IF stages. resolution bandwidth (RBW) in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum
 MINTime argument is Option 200 only

Group Sense commands

Syntax `[SENSe]:DPSA:{BANDwidth|BWIDth}:OPTimization { AUTO | MINTime | MINNoise }`
`[SENSe]:DPSA:{BANDwidth|BWIDth}:OPTimization?`

Related Commands

Arguments `AUTO` optimizes the gain and bandwidth in the RF and IF stages of the RF input circuits.

`MINTime` optimizes the gain and bandwidth to minimize the sweep time.

`MINNoise` optimizes the gain and bandwidth to minimize noise.

Examples `SENSE:DPSA:BANDWIDTH:OPTimization AUTO` automatically sets RBW as a percentage of the Span.

[SENSe]:DPSA:{BANDwidth|BWIDth}[:RESolution]:AUTO

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax [SENSE]:DPSA:{BANDwidth|BWIDth}[:RESOlution]:AUTO { OFF | ON | 0 | 1 }
[SENSE]:DPSA:{BANDwidth|BWIDth}[:RESOlution]:AUTO?

Arguments OFF or 0 specifies that the resolution bandwidth is set manually using the [SENSE]:DPSA:{BANDwidth|BWIDth}:ACTual? command.
ON or 1 specifies that the resolution bandwidth is set automatically.

Examples SENSE:DPSA:BANDWIDTH:AUTO ON sets the resolution bandwidth automatically.

[SENSE]:DPSA:CLEAr:RESuLts (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax [SENSE]:DPSA:CLEAr:RESuLts

Arguments None

Examples SENSE:DPSA:CLEAR:RESULTS restarts multi-trace functions.

[SENSE]:DPSA:COLOr

Sets or queries the color palette of three-dimensional graphs.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax [SENSE]:DPSA:COLOr { RED | GREEN | BLUE | CYAN | BCYan | YELLOW | MAGenta | GRAY | TEMPERature | SPECTra }
[SENSE]:DPSA:COLOr?

Arguments The following table lists the arguments.

Table 2-42: Color palette for DPX spectrum

Argument	Palette
RED	Red
GREen	Green
BLUe	Blue
CYAN	Cyan
BCYan	Binary cyan
YELLow	Yellow
MAGenta	Magenta
GRAY	Gray
TEMPerature	Temperature
SPECtral	Spectral

Examples `SENSE:DPSA:COLOR TEMPerature` selects the temperature color palette.

[SENSe]:DPSA:COLor:MAXimum

Sets or queries the maximum value of the color axis in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax `[SENSe]:DPSA:COLor:MAXimum <value>`
`[SENSe]:DPSA:COLor:MAXimum?`

Arguments `<value> ::= <NRf>` specifies the maximum value of the color axis.
 Range: The minimum value to 100%.
 The minimum value is set using the [\[SENSe\]:DPSA:COLor:MINimum](#) command.

Examples `SENSE:DPSA:COLOR:MAXIMUM 90` sets the maximum value of the color axis to 90%.

[SENSe]:DPSA:COLor:MINimum

Sets or queries the minimum value of the color axis in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax [SENSe]:DPSA:COLor:MINimum <value>
[SENSe]:DPSA:COLor:MINimum?

Arguments <value>::=<Nrf> specifies the minimum value of the color axis.
Range: 0% to the maximum value.

The maximum value is set using the [\[SENSe\]:DPSA:COLor:MAXimum](#) command.

Examples SENSE:DPSA:COLOR:MINIMUM 10 sets the minimum value of the color axis to 10%.

[SENSe]:DPSA:DDENsity:MEASurement:SHOW

Sets the Show measurement value (measurement always visible for DPX Trigger) or queries for the current value.

Conditions Measurement views: DPX spectrum
Option 200 only

Group Sense commands

Syntax [SENSe]:DPSA:DDENsity:MEASurement:SHOW { OFF | ON | 0 | 1 }
[SENSe]:DPSA:DDENsity:MEASurement:SHOW?

Arguments OFF or 0 specifies that the Show measurement value is disabled.
ON or 1 specifies that the Show measurement value is disabled.

Examples SENSE:DPSA:DDENSITY:MEASUREMENT:SHOW ON enables the Show measurement value.

[SENSe]:DPSA:DWELI

Sets or queries the value of the Dwell time for the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum
Option 200 only

Group Sense commands

Syntax [SENSe]:DPSA:DWELI <value>
[SENSe]:DPSA:DWELI?

Arguments <value> ::= <Nrf> specifies the time the DPX sweep remains in a frequency segment collecting data and updating the bitmap and traces before moving on to the next higher frequency segment.
Range: 50 ms to 100 s per frequency segment.

Examples SENSE:DPSA:DWELI 100ms sets the dwell value for sweeps to 100 ms.

[SENSe]:DPSA:DWELI:AUTO

Sets the value of the Dwell time automatically or queries for the current value.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax [SENSe]:DPSA:DWELI:AUTO { OFF | ON | 0 | 1 }
[SENSe]:DPSA:DWELI:AUTO?

Related Commands [\[SENSe\]:DPSA:DWELI](#)

Arguments OFF or 0 specifies that the dwell is set manually.
ON or 1 specifies that the dwell is set automatically.

Examples SENSE:DPSA:DWELI:AUTO ON sets the dwell value automatically for sweeps.

[SENSe]:DPSA:FREQUENCY:CENTer

Sets or queries the center frequency in the DPX spectrum measurement.

NOTE. *The center, start and stop frequencies are set interlocking each other with the following relationships: (start frequency) = (center frequency) - (span)/2 and (stop frequency) = (center frequency) + (span)/2.*

Conditions	Measurement views: DPX spectrum
Group	Sense commands
Syntax	[SENSe]:DPSA:FREQUENCY:CENTer <value> [SENSe]:DPSA:FREQUENCY:CENTer?
Related Commands	[SENSe]:DPSA:FREQUENCY:START , [SENSe]:DPSA:FREQUENCY:STOP
Arguments	<value>::=<NRF> specifies the center frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSe:DPSA:FREQUENCY:CENTer 7.5GHz sets the center frequency to 7.5 GHz.

[SENSe]:DPSA:FREQUENCY:SPAN

Sets or queries the frequency span in the DPX spectrum measurement.

Conditions	Measurement views: DPX spectrum
Group	Sense commands
Syntax	[SENSe]:DPSA:FREQUENCY:SPAN <value> [SENSe]:DPSA:FREQUENCY:SPAN?
Arguments	<value>::=<NRF> is the frequency span. Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110) Option 200 only: <value> is allowed to exceed the maximum real-time bandwidth.

Examples `SENSE:DPSA:FREQUENCY:SPAN 20MHz` sets the span to 20 MHz.

`[SENSe]:DPSA:FREQuency:SPAN:{BANDwidth|BWIDth}[:RESolution]:RATio`

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax `[SENSe]:DPSA:FREQuency:SPAN:{BANDwidth|BWIDth}[:RESolution]:RATio <value>`
`[SENSe]:DPSA:FREQuency:SPAN:{BANDwidth|BWIDth}[:RESolution]:RATio?`

Related Commands [\[SENSe\]:DPSA:{BANDwidth|BWIDth}\[:RESolution\]:AUTO](#)

Arguments `<value>::=<NRF>` is used to calculate the RBW.

Examples `SENSE:DPSA:FREQUENCY:SPAN:BANDWIDTH:RATIO 100` the ratio of 100 is used to set the resolution bandwidth when [\[SENSe\]:DPSA:{BANDwidth|BWIDth}\[:RESolution\]:AUTO](#) is set to ON.

`[SENSe]:DPSA:FREQuency:START`

Sets or queries the measurement start frequency (left edge on the graph) in the DPX spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:DPSA:FREQuency:CENTer](#) command.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax `[SENSe]:DPSA:FREQuency:START <value>`
`[SENSe]:DPSA:FREQuency:START?`

Related Commands [\[SENSe\]:DPSA:FREQuency:STOP](#)

Arguments <value>::=<Nrf> is the measurement start frequency.
Range: (center frequency) ± (span)/2.

Examples SENSE:DPSA:FREQUENCY:START 6.95GHZ sets the start frequency to 6.95 GHz.

[SENSe]:DPSA:FREQuency:STEP

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [SENSe]:DPSA:FREQuency:STEP:AUTO OFF.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax [SENSe]:DPSA:FREQuency:STEP <value>
[SENSe]:DPSA:FREQuency:STEP?

Related Commands [\[SENSe\]:DPSA:FREQuency:STEP:AUTO](#)

Arguments <value>::=<Nrf> specifies the frequency step size.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:DPSA:FREQUENCY:STEP 1.5kHz sets the step size to 1.5 kHz.

[SENSe]:DPSA:FREQuency:STEP:AUTO

Determines whether to set the frequency step size automatically or manually.

Conditions Measurement views: DPX spectrum

Group Sense commands

Syntax	<code>[SENSe]:DPSA:FREQuency:STEP:AUTO { OFF ON 0 1 }</code> <code>[SENSe]:DPSA:FREQuency:STEP:AUTO?</code>
Arguments	OFF or 0 specifies that the frequency step size is set manually using the [SENSe]:DPSA:FREQuency:STEP command. ON or 1 specifies that the frequency step size is set automatically.
Examples	<code>SENSE:DPSA:BANDWIDTH:AUTO ON</code> sets the frequency step size automatically.

[SENSe]:DPSA:FREQuency:STOP

Sets or queries the measurement stop frequency (right edge of the graph) in the DPX spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:DPSA:FREQuency:CENTer](#) command.

Conditions	Measurement views: DPX spectrum
Group	Sense commands
Syntax	<code>[SENSe]:DPSA:FREQuency:STOP <value></code> <code>[SENSe]:DPSA:FREQuency:STOP?</code>
Related Commands	[SENSe]:DPSA:FREQuency:STARt
Arguments	<code><value> ::= <NRf></code> is the measurement stop frequency. Range: (center frequency) \pm (span)/2.
Examples	<code>SENSE:DPSA:FREQUENCY:STOP 7.05GHZ</code> sets the stop frequency to 7.05 GHz.

[SENSe]:DPSA:POINts:COUNT

Sets the number of trace points acquired for the DPX spectrum display.

Conditions	Measurement views: DPX spectrum Option 200 only
-------------------	--

Group	Sense commands
Syntax	[SENSe]:DPSA:POINts:COUnT { P801 P2401 P4001 P10401 } [SENSe]:DPSA:POINts:COUnT?
Arguments	P801 sets the number of sample points to 801. P2401 sets the number of sample points to 2401. P4001 sets the number of sample points to 4001. P8001 sets the number of sample points to 8001. P10401 sets the number of sample points to 10401.
Examples	SENSE:DPSA:POINts:COUnT P2401 sets the number of trace points to acquire for the DPX spectrum display.

[SENSe]:{FM|PM}:BURSt:THReshold

Sets or queries the threshold level above which the input signal is determined to be a burst in the FM/PM measurement. The burst detected first is used for the measurement.

Conditions	Measurement views: FM, PM
Group	Sense commands
Syntax	[SENSe]:{FM PM}:BURSt:THReshold <value> [SENSe]:{FM PM}:BURSt:THReshold?
Arguments	<value> ::= <Nrf> specifies the threshold level. Range: -100.0 to -10.0 dB.
Examples	SENSE:FM:BURSt:THRESHOLD -10 sets the threshold level to -10 dB in the FM measurement.

[SENSe]:{FM|PM}:FREQuency:OFFSet

Sets or queries the carrier frequency offset in the FM/PM measurement.

Conditions	Measurement views: FM, PM
-------------------	---------------------------

Group	Sense commands
Syntax	[SENSE]:{FM PM}:FREQUENCY:OFFSET <value> [SENSE]:{FM PM}:FREQUENCY:OFFSET?
Arguments	<value> ::= <NRf> specifies the frequency offset from the center frequency. Range: $-(\text{MeasBW} * 1.1) / 2$ to $+(\text{MeasBW} * 1.1) / 2$ where MeasBW is set by the command [SENSE]:{AM FM PM}:{BANDwidth BWIDth}:MEASurement.
Examples	SENSE:FM:FREQUENCY:OFFSET 10MHZ sets the carrier frequency offset to 10 MHz.

[SENSE]:{FM|PM}:FREQUENCY:OFFSET:MARKer (No Query Form)

Sets the frequency offset from the selected marker location in the FM measurement.

Sets the frequency offset from the selected delta marker location in the PM measurement.

Conditions	Measurement views: FM, PM
Group	Sense commands
Syntax	[SENSE]:{FM PM}:FREQUENCY:OFFSET:MARKer
Arguments	None.
Examples	SENSE:FM:FREQUENCY:OFFSET:MARKer sets frequency offset from the selected Marker position.

[SENSE]:{FM|PM}:FREQUENCY:SEARCH:AUTO

Determines whether to detect the carrier frequency automatically or manually in the FM/PM measurements.

Conditions	Measurement views: FM, PM
-------------------	---------------------------

Group	Sense commands
Syntax	[SENSE]:{FM PM}:FREQUENCY:SEARCH:AUTO { OFF ON 0 1 } [SENSE]:{FM PM}:FREQUENCY:SEARCH:AUTO?
Arguments	OFF or 0 specifies that the carrier frequency is set manually. Use the command [SENSE]:{FM PM}:FREQUENCY:OFFSet to set the carrier offset frequency. ON or 1 specifies that the carrier frequency is detected automatically.
Examples	SENSE:FM:FREQUENCY:SEARCH:AUTO ON specifies that the carrier frequency is detected automatically.

[SENSE]:FVTime:CLEAr:RESuLts (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Conditions	Measurement views: Frequency versus Time
Group	Sense commands
Syntax	[SENSE]:FVTime:CLEAr:RESuLts
Arguments	None
Examples	SENSE:FVTIME:CLEAR:RESULTS restarts multi-trace functions.

[SENSE]:FVTime:FREQuency:CENTer

Sets or queries the center frequency in the Frequency versus Time measurement.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships: $(start\ frequency) = (center\ frequency) - (span)/2$ and $(stop\ frequency) = (center\ frequency) + (span)/2$.

Conditions	Measurement views: Frequency versus Time
-------------------	--

Group	Sense commands
Syntax	[SENSE]:FVTime:FREQUENCY:CENTer <value> [SENSE]:FVTime:FREQUENCY:CENTer?
Related Commands	[SENSE]:FVTime:FREQUENCY:START , [SENSE]:FVTime:FREQUENCY:STOP
Arguments	<value> ::= <Nrf> specifies the center frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:FVTIME:FREQUENCY:CENTER 7.5GHZ sets the center frequency to 7.5 GHz.

[SENSE]:FVTime:FREQUENCY:SPAN

Sets or queries the frequency span in the Frequency versus Time measurement.

Conditions	Measurement views: Frequency versus Time
Group	Sense commands
Syntax	[SENSE]:FVTime:FREQUENCY:SPAN <value> [SENSE]:FVTime:FREQUENCY:SPAN?
Arguments	<value> ::= <Nrf> is the frequency span. Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)
Examples	SENSE:FVTIME:FREQUENCY:SPAN 20MHZ sets the span to 20 MHz.

[SENSE]:FVTime:FREQUENCY:START

Sets or queries the measurement start frequency (left edge on the graph) in the Frequency versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSE\]:FVTime:FREQUENCY:CENTer](#) command.

Conditions	Measurement views: Frequency versus Time
-------------------	--

Group	Sense commands
Syntax	[SENSe]:FVTime:FREQuency:START <value> [SENSe]:FVTime:FREQuency:START?
Related Commands	[SENSe]:FVTime:FREQuency:STOP
Arguments	<value>::=<Nrf> is the measurement start frequency. Range: (center frequency) ± (span)/2.
Examples	SENSE:FVTIME:FREQUENCY:START 6.95GHZ sets the start frequency to 6.95 GHz.

[SENSe]:FVTime:FREQuency:STEP

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [SENSe]:FVTime:FREQuency:STEP:AUTO OFF.

Conditions	Measurement views: Frequency versus Time
Group	Sense commands
Syntax	[SENSe]:FVTime:FREQuency:STEP <value> [SENSe]:FVTime:FREQuency:STEP?
Related Commands	[SENSe]:FVTime:FREQuency:STEP:AUTO
Arguments	<value>::=<Nrf> specifies the frequency step size. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:FVTIME:FREQUENCY:STEP 1.5kHz sets the step size to 1.5 kHz.

[SENSe]:FVTime:FREQuency:STEP:AUTO

Determines whether to set the frequency step size automatically or manually.

Conditions	Measurement views: Frequency versus Time
Group	Sense commands
Syntax	[SENSe]:FVTime:FREQUENCY:STEP:AUTO { OFF ON 0 1 } [SENSe]:FVTime:FREQUENCY:STEP:AUTO?
Arguments	OFF or 0 specifies that the frequency step size is set manually using the [SENSe]:FVTime:FREQUENCY:STEP command. ON or 1 specifies that the frequency step size is set automatically.
Examples	SENSE:FVTIME:BANDWIDTH:AUTO ON sets the frequency step size automatically.

[SENSe]:FVTime:FREQUENCY:STOP

Sets or queries the measurement stop frequency (right edge of the graph) in the Frequency versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:FVTime:FREQUENCY:CENTer](#) command.

Conditions	Measurement views: Frequency versus Time
Group	Sense commands
Syntax	[SENSe]:FVTime:FREQUENCY:STOP <value> [SENSe]:FVTime:FREQUENCY:STOP?
Related Commands	[SENSe]:FVTime:FREQUENCY:START
Arguments	<value> ::= <Nrf> is the measurement stop frequency. Range: (center frequency) ± (span)/2.
Examples	SENSE:FVTIME:FREQUENCY:STOP 7.05GHZ sets the stop frequency to 7.05 GHz.

[SENSe]:FVTime:MAXTracepoints

Sets or queries the maximum trace points in the Frequency versus Time measurement.

Conditions Measurement views: Frequency versus Time

Group Sense commands

Syntax [SENSe]:FVTime:MAXTracepoints { ONEK | TENK | HUNDredk | NEVERdecimate }
[SENSe]:FVTime:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
TENK sets the maximum trace points to 10 k.
HUNDredk sets the maximum trace points to 100 k.
NEVERdecimate never decimates the trace points.

Examples SENSE:FVTIME:MAXTRACEPOINTS TENK sets the maximum trace points to 10 k.

[SENSe]:IQVTime:CLEAr:RESuLts (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Conditions Measurement views: RF I&Q versus Time

Group Sense commands

Syntax [SENSe]:IQVTime:CLEAr:RESuLts

Arguments None

Examples SENSE:IQVTIME:CLEAR:RESULTS restarts multi-trace functions.

[SENSe]:IQVTime:FREQuency:CENTer

Sets or queries the center frequency in the RF I&Q versus Time measurement.

NOTE. *The center, start and stop frequencies are set interlocking each other with the following relationships: (start frequency) = (center frequency) - (span)/2 and (stop frequency) = (center frequency) + (span)/2.*

Conditions	Measurement views: RF I&Q versus Time
Group	Sense commands
Syntax	[SENSe]:IQVTime:FREQuency:CENTer <value> [SENSe]:IQVTime:FREQuency:CENTer?
Related Commands	[SENSe]:IQVTime:FREQuency:START, [SENSe]:IQVTime:FREQuency:STOP
Arguments	<value> ::= <Nrf> specifies the center frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:IQVTIME:FREQUENCY:CENTER 7.5GHZ sets the center frequency to 7.5 GHz.

[SENSe]:IQVTime:FREQuency:SPAN

Sets or queries the frequency span in the RF I&Q versus Time measurement.

Conditions	Measurement views: RF I&Q versus Time
Group	Sense commands
Syntax	[SENSe]:IQVTime:FREQuency:SPAN <value> [SENSe]:IQVTime:FREQuency:SPAN?
Arguments	<value> ::= <Nrf> is the frequency span. Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)
Examples	SENSE:IQVTIME:FREQUENCY:SPAN 20MHZ sets the span to 20 MHz.

[SENSe]:IQVTime:FREQuency:STARt

Sets or queries the measurement start frequency (left edge on the graph) in the RF I&Q versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:IQVTime:FREQuency:CENTer](#) command.

Conditions	Measurement views: RF I&Q versus Time
Group	Sense commands
Syntax	[SENSe]:IQVTime:FREQuency:STARt <value> [SENSe]:IQVTime:FREQuency:STARt?
Related Commands	[SENSe]:IQVTime:FREQuency:STOP
Arguments	<value>::=<NRF> is the measurement start frequency. Range: (center frequency) ± (span)/2.
Examples	SENSe:IQVTIME:FREQUENCY:STARt 6.95GHZ sets the start frequency to 6.95 GHz.

[SENSe]:IQVTime:FREQuency:STEP

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [\[SENSe\]:IQVTime:FREQuency:STEP:AUTO OFF](#).

Conditions	Measurement views: RF I&Q versus Time
Group	Sense commands
Syntax	[SENSe]:IQVTime:FREQuency:STEP <value> [SENSe]:IQVTime:FREQuency:STEP?
Related Commands	[SENSe]:IQVTime:FREQuency:STEP:AUTO

Arguments <value>::=<Nrf> specifies the frequency step size.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:IQVTIME:FREQUENCY:STEP 1.5kHz sets the step size to 1.5 kHz.

[SENSe]:IQVTime:FREQuency:STEP:AUTO

Determines whether to set the frequency step size automatically or manually.

Conditions Measurement views: RF I&Q versus Time

Group Sense commands

Syntax [SENSe]:IQVTime:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[SENSe]:IQVTime:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the [\[SENSe\]:IQVTime:FREQuency:STEP](#) command.

ON or 1 specifies that the frequency step size is set automatically.

Examples SENSE:IQVTIME:FREQUENCY:STEP:AUTO ON sets the frequency step size automatically.

[SENSe]:IQVTime:FREQuency:STOP

Sets or queries the measurement stop frequency (right edge of the graph) in the RF I&Q versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:IQVTime:FREQuency:CENTer](#) command.

Conditions Measurement views: RF I&Q versus Time

Group Sense commands

Syntax [SENSe]:IQVTime:FREQuency:STOP <value>
[SENSe]:IQVTime:FREQuency:STOP?

Related Commands [\[SENSe\]:IQVTime:FREQuency:STARt](#)

Arguments <value>::=<NRF> is the measurement stop frequency.
Range: (center frequency) ± (span)/2.

Examples SENSE:IQVTIME:FREQUENCY:STOP 7.05GHZ sets the stop frequency to 7.05 GHz.

[SENSe]:IQVTime:MAXTracepoints

Sets or queries the maximum trace points in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Sense commands

Syntax [SENSe]:IQVTime:MAXTracepoints { ONEK | TENK | HUNDredk | NEVERdecimate }
[SENSe]:IQVTime:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
TENK sets the maximum trace points to 10 k.
HUNDredk sets the maximum trace points to 100 k.
NEVERdecimate never decimates the trace points.

Examples SENSE:IQVTIME:MAXTRACEPOINTS TENK sets the maximum trace points to 10 k.

[SENSe]:MCPower:AVERAge

Sets or queries the average method in the MCPR measurement.

Conditions Measurement views: MCPR

Group Sense commands

Syntax	<code>[SENSe]:MCPower:AVERAge { OFF TIME FREQuency }</code> <code>[SENSe]:MCPower:AVERAge?</code>
Arguments	OFF disables averaging. TIME performs averaging for time samples. FREQuency performs averaging for frequency samples.
Examples	<code>SENSE:MCPOWER:AVERAGE TIME</code> performs averaging for time samples.

[SENSe]:MCPower:AVERAge:COUNT

Sets or queries the average count in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	<code>[SENSe]:MCPower:AVERAge:COUNT <value></code> <code>[SENSe]:MCPower:AVERAge:COUNT?</code>
Arguments	<code><value> ::= <NR1></code> specifies the average count. Range: 2 to 10000.
Examples	<code>SENSE:MCPOWER:AVERAGE:COUNT 256</code> sets the average count to 256.

[SENSe]:MCPower:{BANDwidth|BWIDth}[:RESolution]

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets `[SENSe]:MCPower{BANDwidth|BWIDth}[:RESolution]:AUTO OFF`.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	<code>[SENSe]:MCPower:{BANDwidth BWIDth}[:RESolution] <value></code> <code>[SENSe]:MCPower:{BANDwidth BWIDth}[:RESolution]?</code>

Related Commands [\[SENSe\]:MCPower:{BANDwidth|BWIDth}\[:RESolution\]:AUTO](#)

Arguments <value>::=<NRF> specifies the RBW. Range: 100 Hz to 5 MHz.

Examples SENSE:MCPOWER:BANDWIDTH:RESOLUTION 200kHz sets the RBW to 200 kHz.

[SENSe]:MCPower:{BANDwidth|BWIDth}[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the MCPR measurement.

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:{BANDwidth|BWIDth}[:RESolution]:ACTual?

Arguments None

Returns <NRF> The actual RBW in Hz.

Examples SENSE:MCPOWER:BANDWIDTH:RESOLUTION:ACTUAL? might return 299.624E+3, indicating that the actual RBW is 299.624 kHz.

[SENSe]:MCPower:{BANDwidth|BWIDth}[:RESolution]:AUTO

Determines whether to set the resolution bandwidth (RBW) automatically or manually.

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:{BANDwidth|BWIDth}[:RESolution]:AUTO { OFF | ON | 0 | 1 }
[SENSe]:MCPower:{BANDwidth|BWIDth}[:RESolution]:AUTO?

Arguments	OFF or 0 specifies that the resolution bandwidth is set manually using the <code>[SENSe]:MCPower:{BANDwidth BWIDth}[:RESolution]</code> command. ON or 1 specifies that the resolution bandwidth is set automatically.
Examples	<code>SENSE:MCPOWER:BANDWIDTH:AUTO ON</code> sets the resolution bandwidth automatically.

`[SENSe]:MCPower:{BANDwidth|BWIDth}:VIDeo`

Sets or queries the video bandwidth (VBW). Programming a specified VBW sets `[SENSe]:MCPower:{BANDwidth|BWIDth}:VIDeo:STATE` OFF.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	<code>[SENSe]:MCPower:{BANDwidth BWIDth}:VIDeo <value></code> <code>[SENSe]:MCPower:{BANDwidth BWIDth}:VIDeo?</code>
Related Commands	<code>[SENSe]:MCPower:{BANDwidth BWIDth}:VIDeo:STATE</code>
Arguments	<code><value>::=<Nrf></code> specifies the VBW. Range: Current RBW/10 ⁴ (1 Hz minimum) to Current RBW.
Examples	<code>SENSE:MCPOWER:BANDWIDTH:VIDEO 200kHz</code> sets the VBW to 200 kHz.

`[SENSe]:MCPower:{BANDwidth|BWIDth}:VIDeo:STATE`

Determines whether to enable the video bandwidth (VBW) in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	<code>[SENSe]:MCPower:{BANDwidth BWIDth}:VIDeo:STATE { OFF ON 0 1 }</code>

[SENSe]:MCPower:{BANDwidth|BWIDth}:VIDeo:STATE?

Arguments OFF or 0 disables the VBW.
ON or 1 enables the VBW.

Examples SENSE:MCPOWER:BANDWIDTH:VIDEO:STATE ON enables the VBW.

[SENSe]:MCPower:CHANnel:ADJacent:ADD (No Query Form)

Adds a pair of upper and lower adjacent channels in the MCPR measurement.

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:CHANnel:ADJacent:ADD <offset>, <bandwidth>

Arguments <offset>::=<Nrf> specifies the offset from the center frequency for the adjacent channel. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
<bandwidth>::=<Nrf> specifies the bandwidth of the adjacent channel. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:MCPOWER:CHANNEL:ADJACENT:ADD 200kHz,80kHz adds a pair of upper and lower adjacent channels with the offset of ± 200 kHz and the bandwidth of 80 kHz.

[SENSe]:MCPower:CHANnel:ADJacent:DELeTe (No Query Form)

Deletes a selected adjacent channel in the MCPR measurement.

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:CHANnel:ADJacent:DELeTe <channel>

Arguments	<code><channel>::=<string></code> specifies the channel to be deleted. Specify the channel with "A<n>" for the adjacent channel where <n> represents the channel number (<n> = 1, 2, 3,...). See the example below.
Examples	<code>SENSE:MCPower:CHANNEL:ADJacent:DELeTe "A2"</code> deletes A2 (the adjacent channel 2).

[SENSE]:MCPower:CHANnel:FILTer

Sets or queries the adjacent channel filter in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	<code>[SENSE]:MCPower:CHANnel:FILTer { RRCosine NONE }</code> <code>[SENSE]:MCPower:CHANnel:FILTer?</code>
Arguments	<code>RRCosine</code> selects the Root-Raised-Cosine filter. <code>NONE</code> uses no filter.
Examples	<code>SENSE:MCPOWER:CHANNEL:FILTER RRCosine</code> selects Root-Raised-Cosine for the adjacent channel filter.

[SENSE]:MCPower:CHANnel:MAIN:{BANDwidth|BWIDth}

Sets or queries the frequency bandwidth of the main channels (all share the same value) in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	<code>[SENSE]:MCPower:CHANnel:MAIN:{BANDwidth BWIDth} <value></code> <code>[SENSE]:MCPower:CHANnel:MAIN:{BANDwidth BWIDth}?</code>

Arguments <value>::=<NRF> specifies the main channel bandwidth.
Range: 1 Hz to full span.

Examples SENSE:MCPOWER:CHANNEL:MAIN:BANDWIDTH 4.5MHZ sets the main channel bandwidth to 4.5 MHz.

[SENSe]:MCPower:CHANnel:MAIN:COUNT

Sets or queries the number of main channels in the MCPR measurement. You can use this command to add and remove main channels.

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:CHANnel:MAIN:COUNT <value>
[SENSe]:MCPower:CHANnel:MAIN:COUNT?

Arguments <value>::=<NRF> specifies the number of main channels. Range: 1 to 99.

Examples SENSE:MCPOWER:CHANNEL:MAIN:COUNT 3 sets the the number of main channels to 3.

[SENSe]:MCPower:CHANnel:MAIN:INACTive

Makes a specified main channel inactive. You can set it on or off. The query returns all inactive main channels.

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:CHANnel:MAIN:INACTive <channel>,<boolean>
[SENSe]:MCPower:CHANnel:MAIN:INACTive?

Arguments <channel>::=<string> specifies the channel to be inactive.
Specify the channel with "M<n>" for the main channel where <n> represents the channel number (<n> = 1, 2, 3,...). See the example below.

<boolean> ::= { OFF | ON | 0 | 1 } specifies that the specified channel is inactive (On) or not (Off).

Examples SENSE:MCPOWER:CHANNEL:MAIN:INACTIVE "M2", ON makes the main channel 2 inactive.

[SENSe]:MCPower:CHANnel:MAIN:SPACing

Sets or queries frequency difference between centers of each main channel in the MCPR measurement.

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:CHANnel:MAIN:SPACing <value>
[SENSe]:MCPower:CHANnel:MAIN:SPACing?

Arguments <value> ::= <Nrf> specifies the spacing between two adjacent main channels. Range: 1 Hz to 1 GHz.

Examples SENSE:MCPOWER:CHANNEL:MAIN:SPACING 5MHZ sets the main channel spacing to 5 MHz.

[SENSe]:MCPower:CHIPrate

Sets or queries the chip rate in the MCPR measurement. This command is valid when [\[SENSe\]:MCPower:CHANnel:FILTer](#) is set to RRCosine (Root-Raised-Cosine).

Conditions Measurement views: MCPR

Group Sense commands

Syntax [SENSe]:MCPower:CHIPrate <value>
[SENSe]:MCPower:CHIPrate?

Arguments <value> ::= <Nrf> specifies the chip rate. Range: 100 Hz to 105 MHz.

Examples `SENSE:MCPOWER:CHIPRATE 1kHz` sets the chip rate to 1 kHz.

[SENSe]:MCPower:CLEAr:RESuLts (No Query Form)

Restarts the average trace.

Conditions Measurement views: MCPR

Group Sense commands

Syntax `[SENSe]:MCPower:CLEAr:RESuLts`

Arguments None

Examples `SENSE:MCPOWER:CLEAR:RESULTS` restarts the average trace.

[SENSe]:MCPower:FREQuency

Sets or queries the center frequency in the MCPR measurement.

Conditions Measurement views: MCPR

Group Sense commands

Syntax `[SENSe]:MCPower:FREQuency <value>`
`[SENSe]:MCPower:FREQuency?`

Arguments `<value>::=<nrf>` specifies the center frequency.
 Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples `SENSE:MCPOWER:FREQUENCY 2.35GHz` sets the center frequency to 2.35 GHz.

[SENSe]:MCPower:FREQuency:STEP

Sets or queries the frequency step size. Programming a specified step size sets `[SENSe]:MCPower:FREQuency:STEP:AUTO OFF`.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	[SENSe]:MCPower:FREQUENCY:STEP <value> [SENSe]:MCPower:FREQUENCY:STEP?
Related Commands	[SENSe]:MCPower:FREQUENCY:STEP:AUTO
Arguments	<value> ::= <Nrf> specifies the frequency step size. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:MCPOWER:FREQUENCY:STEP 50kHz sets the frequency step size to 50 kHz.

[SENSe]:MCPower:FREQUENCY:STEP:AUTO

Determines whether to set the frequency step size automatically or manually in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	[SENSe]:MCPower:FREQUENCY:STEP:AUTO { OFF ON 0 1 } [SENSe]:MCPower:FREQUENCY:STEP:AUTO?
Arguments	OFF or 0 specifies that the frequency step size is set manually using the [SENSe]:MCPower:FREQUENCY:STEP command. ON or 1 specifies that the frequency step size is set automatically.
Examples	SENSE:MCPOWER:FREQUENCY:STEP:AUTO ON specifies that the frequency step size is set automatically.

[SENSe]:MCPower:NFLoor:STATe

Determines whether to enable correction for noise floor.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	[SENSe]:MCPower:NFLoor:STATE { OFF ON 0 1 } [SENSe]:MCPower:NFLoor:STATE?
Arguments	OFF or 0 disables correction for noise floor. ON or 1 enables correction for noise floor.
Examples	SENSE:MCPOWER:NFLOOR:STATE ON enables correction for noise floor.

[SENSe]:MCPower:OPTimize:SPAN

Sets or queries the optimization method in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	[SENSe]:MCPower:OPTimize:SPAN { RTBandwidth DRANge } [SENSe]:MCPower:OPTimize:SPAN?
Arguments	RTBandwidth optimizes the measurement for real-time bandwidth. DRANge optimizes the measurement for dynamic range.
Examples	SENSE:MCPOWER:OPTIMIZE:SPAN RTBandwidth optimizes the measurement for real-time bandwidth.

[SENSe]:MCPower:POINts:COUNT

Sets or queries the number of trace points in the MCPR display.

Conditions	Measurement views: MCPR
Group	Sense commands

Syntax	<code>[SENSe]:MCPower:POINts:COUnT { P801 P2401 P4001 P8001 P10801 }</code> <code>[SENSe]:MCPower:POINts:COUnT?</code>
Arguments	P801 P2401 P4001 P8001 P10801 set the number of trace points.
Examples	<code>SENSE:MCPOWER:POINTS:COUNT P4001</code> sets the number of trace points in the MCPR measurement to 4001.

[SENSe]:MCPower:RCHannels? (Query Only)

Queries the power reference in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	<code>[SENSe]:MCPower:RCHannels?</code>
Arguments	None
Returns	<code><power_ref>::={ Total M<x> }</code> where <code><x> = 1 to 99</code> . <code>Total</code> indicates that the power reference is the total power of all the active channels. <code>M<x></code> indicates that the power reference is the main channel with the index (<code><x></code>).
Examples	<code>SENSE:MCPOWER:RCHANNELS?</code> might return <code>M3</code> , indicating that the power reference is the main channel 3.

[SENSe]:MCPower:RCHannels:MAIN<x> (No Query Form)

Sets the power reference to the main channel with the index (`<x>`) in the MCPR measurement.

The parameter `<x> = 1 to 99`, representing the main channel 1 to 99, respectively. The main channel must be defined using the `[SENSe]:MCPower:CHANnel:MAIN` commands.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	[SENSE]:MCPower:RChannels:MAIN<x>
Related Commands	[:SENSE]:MCPower:CHANnel:MAIN commands
Arguments	None
Examples	SENSE:MCPOWER:RCHANNELS:MAIN3 selects Main 3 for the power reference channel.

[SENSE]:MCPower:RChannels:TOTal (No Query Form)

Sets the power reference to the total power of all the active channels in the MCPR measurement.

Conditions	Measurement views: MCPR
Group	Sense commands
Syntax	[SENSE]:MCPower:RChannels:TOTal
Arguments	None
Examples	SENSE:MCPOWER:RCHANNELS:TOTAL sets the power reference to the total power of all the active channels.

[SENSE]:MCPower:RRCRolloff

Sets or queries the filter parameter (roll-off ratio) for the Root Raised Cosine filter.

Conditions	Measurement views: MCPR
Group	Sense commands

Syntax [SENSe]:MCPower:RRCRo1loff <value>
[SENSe]:MCPower:RRCRo1loff?

Related Commands [SENSe]:MCPower:CHANnel:FILTer

Arguments <value> ::= <Nrf> specifies the filter parameter.
Range: 0.001 to 1, 0.0001 step.

Examples SENSE:MCPOWER:RRCROLLOFF 0.3 sets the filter parameter to 0.3.

[SENSe]:MEASurement:FREQuency

Sets or queries the measurement frequency.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:MEASurement:FREQuency <value>
[SENSe]:MEASurement:FREQuency?

Arguments <value> ::= <Nrf> specifies the measurement frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:MEASUREMENT:FREQUENCY 7.5GHZ sets the measurement frequency to 7.5 GHz.

[SENSe]:MEASurement:FREQuency:CENTer:LOCK

Sets or queries locking the measurement center frequency.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:MEASurement:FREQuency:CENTer:LOCK { OFF | ON | 0 | 1 }

[SENSE]:MEASUREMENT:FREQUENCY:CENTER:LOCK?

Arguments OFF or 0 disables locking the center frequency.
ON or 1 enables locking the center frequency.

Examples [SENSE]:MEASUREMENT:FREQUENCY:CENTER:LOCK ON locks the center frequency.

[SENSE]:OBWidth:AVERage

Sets or queries whether to enable averaging in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax [SENSE]:OBwidth:AVERage { OFF | ON | 0 | 1 }
[SENSE]:OBwidth:AVERage?

Arguments OFF or 0 disables averaging.
ON or 1 enables averaging.

Examples SENSE:OBWIDTH:AVERAGE ON enables averaging.

[SENSE]:OBWidth:AVERage:COUNT

Sets or queries the number of measurements for averaging in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax [SENSE]:OBwidth:AVERage:COUNT <number>
[SENSE]:OBwidth:AVERage:COUNT?

Arguments <number> ::= <NR1> specifies the average count. Range: 2 to 10000.

Examples SENSE:OBWIDTH:AVERAGE:COUNT 64 sets the average count to 64.

[SENSE]:OBWidth:{BANDwidth|BWIDth}:MEASurement

Sets or queries the measurement bandwidth to determine the total power in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax [SENSE]:OBwidth:{BANDwidth|BWIDth}:MEASurement <value>
[SENSE]:OBwidth:{BANDwidth|BWIDth}:MEASurement?

Arguments <value> ::= <NRf> specifies the measurement bandwidth.
Range: 100 Hz to 109 MHz.

Examples SENSE:OBWIDTH:BANDWIDTH:MEASUREMENT 10MHZ sets the measurement bandwidth to 10 MHz.

[SENSE]:OBWidth:{BANDwidth|BWIDth}[:RESolution]

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [SENSE]:OBWidth{BANDwidth|BWIDth}[:RESolution]:AUTO OFF.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax [SENSE]:OBwidth:{BANDwidth|BWIDth}[:RESolution] <value>
[SENSE]:OBwidth:{BANDwidth|BWIDth}[:RESolution]?

Related Commands [SENSE]:OBWidth:{BANDwidth|BWIDth}[:RESolution]:AUTO

Arguments <value> ::= <NRf> specifies the RBW. Range: 100 Hz to 5 MHz.

Examples `SENSE:OBWIDTH:BANDWIDTH:RESOLUTION 200kHz` sets the RBW to 200 kHz.

[SENSe]:OBWidth:{BANDwidth|BWIDth}[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax `[SENSe]:OBwidth:{BANDwidth|BWIDth}[:RESolution]:ACTual?`

Arguments None

Returns <NRF> The actual RBW in Hz.

Examples `SENSE:OBWIDTH:BANDWIDTH:RESOLUTION:ACTUAL?` might return `299.624E+3`, indicating that the actual RBW is 299.624 kHz.

[SENSe]:OBWidth:{BANDwidth|BWIDth}[:RESolution]:AUTO

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax `[SENSe]:OBwidth:{BANDwidth|BWIDth}[:RESolution]:AUTO { OFF | ON | 0 | 1 }`
`[SENSe]:OBwidth:{BANDwidth|BWIDth}[:RESolution]:AUTO?`

Arguments OFF or 0 specifies that the RBW is set manually using the `[SENSe]:OBWidth:{BANDwidth|BWIDth}[:RESolution]` command.

ON or 1 specifies that the RBW is set automatically.

Examples `SENSE:OBWIDTH:BANDWIDTH:AUTO ON` sets the RBW automatically.

[SENSe]:OBWidth:{BANDwidth|BWIDth}:VIDeo

Sets or queries the video bandwidth (VBW). Programming a specified VBW sets `[SENSe]:OBWidth{BANDwidth|BWIDth}:VIDeo:STATe OFF`.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax `[SENSe]:OBwidth:{BANDwidth|BWIDth}:VIDeo <value>`
`[SENSe]:OBwidth:{BANDwidth|BWIDth}:VIDeo?`

Arguments `<value>::=<NRf>` specifies the VBW.
 Range: Current RBW/10⁴ (1 Hz minimum) to Current RBW.

Examples `SENSE:OBWIDTH:BANDWIDTH:VIDEO 200kHz` sets the VBW to 200 kHz.

[SENSe]:OBWidth:{BANDwidth|BWIDth}:VIDeo:STATe

Determines whether to enable the video bandwidth (VBW) in the Occupied Bandwidth measurement.

Conditions Measurement views: Occupied Bandwidth

Group Sense commands

Syntax `[SENSe]:OBwidth:{BANDwidth|BWIDth}:VIDeo:STATe { OFF | ON`
`| 0 | 1 }`
`[SENSe]:OBwidth:{BANDwidth|BWIDth}:VIDeo:STATe?`

Arguments OFF or 0 disables the VBW.
 ON or 1 enables the VBW.

Examples `SENSE:OBWIDTH:BANDWIDTH:VIDEO:STATE ON` enables the VBW.

[SENSE]:OBWidth:CLEar:RESuLts (No Query Form)

Restarts the average trace. This command is valid when [SENSE]:OBWidth:AVERage is set to ON.

Conditions	Measurement views: Occupied Bandwidth
Group	Sense commands
Syntax	[SENSE]:OBwidth:CLEar:RESuLts
Arguments	None
Examples	SENSE:OBWIDTH:CLEAR:RESULTS restarts the average trace.

[SENSE]:OBWidth:FREQuency:CENTer

Sets or queries the center frequency in the Occupied Bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Sense commands
Syntax	[SENSE]:OBwidth:FREQuency:CENTer <value> [SENSE]:OBwidth:FREQuency:CENTer?
Arguments	<value> ::= <Nrf> specifies the center frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:OBWIDTH:FREQUENCY:CENTER 7.5GHZ sets the center frequency to 7.5 GHz.

[SENSE]:OBWidth:FREQuency:STEP

Sets or queries the frequency step size in the Occupied Bandwidth measurement. Programming a specified step size sets [SENSE]:OBWidth:FREQuency:STEP AUTO OFF.

Conditions	Measurement views: Occupied Bandwidth
Group	Sense commands
Syntax	[SENSe]:OBWidth:FREQUENCY:STEP <value> [SENSe]:OBWidth:FREQUENCY:STEP?
Related Commands	[SENSe]:OBWidth:FREQUENCY:STEP:AUTO
Arguments	<value> ::= <Nrf> specifies the frequency step size. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:OBWIDTH:FREQUENCY:STEP 1kHz sets the frequency step size to 1 kHz.

[SENSe]:OBWidth:FREQUENCY:STEP:AUTO

Determines whether to set the frequency step size automatically or manually in the Occupied Bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Sense commands
Syntax	[SENSe]:OBWidth:FREQUENCY:STEP:AUTO { OFF ON 0 1 } [SENSe]:OBWidth:FREQUENCY:STEP:AUTO?
Arguments	OFF or 0 specifies that the frequency step size is set manually using the [SENSe]:OBWidth:FREQUENCY:STEP command. ON or 1 specifies that the frequency step size is set automatically.
Examples	SENSE:OBWIDTH:FREQUENCY:STEP:AUTO ON specifies that the frequency step size is set automatically.

[SENSe]:OBWidth:PERCent

Sets or queries the occupied bandwidth percent power (power ratio of the occupied bandwidth to the measurement bandwidth).

Conditions	Measurement views: Occupied Bandwidth
Group	Sense commands
Syntax	[SENSE]:OBwidth:PERCent <value> [SENSE]:OBwidth:PERCent?
Arguments	<value>::=<NRF> specifies the occupied bandwidth percent power. Range: 50 to 99.9%.
Examples	SENSE:OBWIDTH:PERCENT 98 sets the occupied bandwidth percent power to 98%.

[SENSE]:OBWidth:XDBLevel

Sets or queries the x dB level (how far down from the peak level the bandwidth is measured) in the x dB bandwidth measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Sense commands
Syntax	[SENSE]:OBwidth:XDBLevel <value> [SENSE]:OBwidth:XDBLevel?
Arguments	<value>::=<NRF> specifies the x dB level. Range: -80 to -1 dB.
Examples	SENSE:OBWIDTH:XDBLEVEL -10 sets the x dB level to -10 dB.

[SENSE]:PHVTime:CLEar:RESults (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Conditions	Measurement views: Phase versus Time
Group	Sense commands

Syntax	<code>[SENSe]:PHVTime:CLEAr:RESuLts</code>
Arguments	None
Examples	<code>SENSE:PHVTIME:CLEAR:RESULTS</code> restarts multi-trace functions.

[SENSe]:PHVTime:FREQuency:CENTer

Sets or queries the center frequency in the Phase versus Time measurement.

NOTE. *The center, start and stop frequencies are set interlocking each other with the following relationships: (start frequency) = (center frequency) - (span)/2 and (stop frequency) = (center frequency) + (span)/2.*

Conditions	Measurement views: Phase versus Time
Group	Sense commands
Syntax	<code>[SENSe]:PHVTime:FREQuency:CENTer <value></code> <code>[SENSe]:PHVTime:FREQuency:CENTer?</code>
Related Commands	[SENSe]:PHVTime:FREQuency:START , [SENSe]:PHVTime:FREQuency:STOP
Arguments	<code><value> ::= <NRF></code> specifies the center frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	<code>SENSE:PHVTIME:FREQUENCY:CENTER 7.5GHZ</code> sets the center frequency to 7.5 GHz.

[SENSe]:PHVTime:FREQuency:SPAN

Sets or queries the frequency span in the Phase versus Time measurement.

Conditions	Measurement views: Phase versus Time
Group	Sense commands

Syntax [SENSe]:PHVTime:FREQuency:SPAN <value>
[SENSe]:PHVTime:FREQuency:SPAN?

Arguments <value>::=<NRF> is the frequency span.
Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)

Examples SENSE:PHVTIME:FREQUENCY:SPAN 20MHZ sets the span to 20 MHz.

[SENSe]:PHVTime:FREQuency:START

Sets or queries the measurement start frequency (left edge on the graph) in the Phase versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:PHVTime:FREQuency:CENTer](#) command.

Conditions Measurement views: Phase versus Time

Group Sense commands

Syntax [SENSe]:PHVTime:FREQuency:START <value>
[SENSe]:PHVTime:FREQuency:START?

Related Commands [\[SENSe\]:PHVTime:FREQuency:STOP](#)

Arguments <value>::=<NRF> is the measurement start frequency.
Range: (center frequency) ± (span)/2.

Examples SENSE:PHVTIME:FREQUENCY:START 6.95GHZ sets the start frequency to 6.95 GHz.

[SENSe]:PHVTime:FREQuency:STEP

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [\[SENSe\]:PHVTime:FREQuency:STEP:AUTO OFF](#).

Conditions Measurement views: Phase versus Time

Group	Sense commands
Syntax	[SENSe]:PHVTime:FREQuency:STEP <value> [SENSe]:PHVTime:FREQuency:STEP?
Related Commands	[SENSe]:PHVTime:FREQuency:STEP:AUTO
Arguments	<value> ::= <Nrf> specifies the frequency step size. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:PHVTIME:FREQUENCY:STEP 1.5kHz sets the step size to 1.5 kHz.

[SENSe]:PHVTime:FREQuency:STEP:AUTO

Determines whether to set the frequency step size automatically or manually.

Conditions	Measurement views: Phase versus Time
Group	Sense commands
Syntax	[SENSe]:PHVTime:FREQuency:STEP:AUTO { OFF ON 0 1 } [SENSe]:PHVTime:FREQuency:STEP:AUTO?
Arguments	OFF or 0 specifies that the frequency step size is set manually using the [SENSe]:PHVTime:FREQuency:STEP command. ON or 1 specifies that the frequency step size is set automatically.
Examples	SENSE:PHVTIME:BANDWIDTH:AUTO ON sets the frequency step size automatically.

[SENSe]:PHVTime:FREQuency:STOP

Sets or queries the measurement stop frequency (right edge of the graph) in the Phase versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [SENSe]:PHVTime:FREQuency:CENTer command.

Conditions	Measurement views: Phase versus Time
Group	Sense commands
Syntax	[SENSe]:PHVTime:FREQUENCY:STOP <value> [SENSe]:PHVTime:FREQUENCY:STOP?
Related Commands	[SENSe]:PHVTime:FREQUENCY:START
Arguments	<value> ::= <NRF> is the measurement stop frequency. Range: (center frequency) ± (span)/2.
Examples	SENSE:PHVTIME:FREQUENCY:STOP 7.05GHZ sets the stop frequency to 7.05 GHz.

[SENSe]:PHVTime:MAXTracepoints

Sets or queries the maximum trace points in the Phase versus Time measurement.

Conditions	Measurement views: Phase versus Time
Group	Sense commands
Syntax	[SENSe]:PHVTime:MAXTracepoints { ONEK TENK HUNDredk NEVERdecimate } [SENSe]:PHVTime:MAXTracepoints?
Arguments	ONEK sets the maximum trace points to 1 k. TENK sets the maximum trace points to 10 k. HUNDredk sets the maximum trace points to 100 k. NEVERdecimate never decimates the trace points.
Examples	SENSE:PHVTIME:MAXTRACEPOINTS TENK sets the maximum trace points to 10 k.

[SENSe]:PM:PHASe:OFFSet

Sets or queries the phase offset in the PM measurement.

Conditions Measurement views: PM

Group Sense commands

Syntax [SENSe]:PM:PHASe:OFFSet <value>
[SENSe]:PM:PHASe:OFFSet?

Arguments <value>::=<Nrf> specifies the phase offset. Range: -180 to +180 °.

Examples SENSE:PM:PHASE:OFFSET 10deg sets the phase offset to 10 °.

[SENSe]:PM:PHASe:OFFSet:MARKer (No Query Form)

Sets the phase offset from the selected marker location in the PM measurement.

Conditions Measurement views: PM

Group Sense commands

Syntax [SENSe]:PM:PHASe:OFFSet:MARKer

Arguments None.

Examples SENSE:PM:PHASE:OFFSET:MARKER sets the phase offset from the selected Marker position.

[SENSe]:PM:PHASe:SEARch:AUTO

Determines whether to detect the phase automatically or manually in the PM measurement.

Conditions Measurement views: PM

Group	Sense commands
Syntax	[SENSE]:PM:PHASE:SEARCH:AUTO { OFF ON 0 1 } [SENSE]:PM:PHASE:SEARCH:AUTO?
Arguments	OFF or 0 specifies that the phase offset is set manually using the command [SENSE]:PM:PHASE:OFFSet. ON or 1 specifies that the phase is detected automatically.
Examples	SENSE:PM:PHASE:SEARCH:AUTO ON specifies that the phase is detected automatically.

[SENSE]:PNOise:AVERage:COUNT

Sets or queries the number of traces to combine for averaging in the phase noise measurement. This command is effective when [SENSE]:PNOise:AVERage:ENABLE is set to ON.

Conditions	Measurement views: Phase noise
Group	Sense commands
Syntax	[SENSE]:PNOise:AVERage:COUNT <number> [SENSE]:PNOise:AVERage:COUNT?
Arguments	<number> ::= <NR1> specifies the average count. Range: 2 to 10000.
Examples	SENSE:PNOISE:AVERAGE:COUNT 64 sets the average count to 64.

[SENSE]:PNOise:AVERage:ENABLE

Determines whether to enable averaging trace in the phase noise measurement.

Conditions	Measurement views: Phase noise
Group	Sense commands

Syntax	<code>[SENSE]:PNOise:AVERAge:ENABle { OFF ON 0 1 }</code> <code>[SENSE]:PNOise:AVERAge:ENABle?</code>
Arguments	OFF disables averaging trace. ON enables averaging trace.
Examples	<code>SENSE:PNOISE:AVERAGE:ENABLE ON</code> enables averaging trace.

[SENSE]:PNOise:CARRier:FREQUency:TRACk

Determines whether to enable or disable tracking the carrier frequency in the phase noise measurement.

Conditions	Measurement views: Phase noise
Group	Sense commands
Syntax	<code>[SENSE]:PNOise:CARRier:FREQUency:TRACk { OFF ON 0 1 }</code> <code>[SENSE]:PNOise:CARRier:FREQUency:TRACk?</code>
Arguments	OFF or 0 disables tracking the carrier frequency. ON or 1 enables tracking the carrier frequency.
Examples	<code>SENSE:PNOISE:CARRIER:FREQUENCY:TRACK ON</code> enables tracking the carrier frequency.

[SENSE]:PNOise:CARRier:THReshold

Sets or queries the threshold level to detect the carrier in the phase noise measurement.

Conditions	Measurement views: Phase noise
Group	Sense commands
Syntax	<code>[SENSE]:PNOise:CARRier:THReshold <value></code> <code>[SENSE]:PNOise:CARRier:THReshold?</code>

Arguments <value>::=<Nrf> specifies the threshold level above which the input signal is determined to be a carrier. Range: -60 to 0 dBm.

Examples SENSE:PNOISE:CARRIER:THRESHOLD -25 sets the carrier threshold level to -25 dB.

[SENSE]:PNOISE:CLEAR:RESULTS (No Query Form)

Restarts the average process, clearing average data and counter.

Conditions Measurement views: Phase noise

Group Sense commands

Syntax [SENSE]:PNOISE:CLEAR:RESULTS

Arguments None

Examples SENSE:PNOISE:CLEAR:RESULTS restarts the average process.

[SENSE]:PNOISE:FREQUENCY:INTEGRATION:OFFSET:START

Sets or queries the start offset frequency for integration in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Sense commands

Syntax [SENSE]:PNOISE:FREQUENCY:INTEGRATION:OFFSET:START <value>
[SENSE]:PNOISE:FREQUENCY:INTEGRATION:OFFSET:START?

Arguments <value>::=<Nrf> specifies the start offset frequency for integration. It must be less than the stop offset frequency. Range: 10 Hz to Stop Offset Frequency - 1 Hz.

Examples `SENSE:PNOISE:FREQUENCY:INTEGRATION:OFFSET:START 100kHz` sets the start offset frequency for integration to 100 kHz.

[SENSe]:PNOise:FREQuency:INTEgration:OFFSet:STOP

Sets or queries the stop offset frequency for integration in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Sense commands

Syntax `[SENSe]:PNOise:FREQuency:INTEgration:OFFSet:STOP <value>`
`[SENSe]:PNOise:FREQuency:INTEgration:OFFSet:STOP?`

Arguments `<value>::=<Nrf>` specifies the stop offset frequency for integration. It must be greater than the start offset frequency.
 Range: 11 Hz to 1 GHz.

Examples `SENSE:PNOISE:FREQUENCY:INTEGRATION:OFFSET:STOP 100MHZ` sets the stop offset frequency for integration to 100 MHz.

[SENSe]:PNOise:FREQuency:PLOT:OFFSet:START

Sets or queries the start offset frequency for plotting the phase noise trace.

Conditions Measurement views: Phase noise

Group Sense commands

Syntax `[SENSe]:PNOise:FREQuency:PLOT:OFFSet:START <value>`
`[SENSe]:PNOise:FREQuency:PLOT:OFFSet:START?`

Arguments `<value>::=<Nrf>` specifies the start offset frequency for the trace plot. It must be less than the stop offset frequency.
 Range: 10 Hz to 100 MHz in a tenfold sequence.

Examples `SENSE:PNOISE:FREQUENCY:PLOT:OFFSET:START 100kHz` sets the start offset frequency for plot to 100 kHz.

[SENSe]:PNOise:FREQuency:PLOT:OFFSet:STOP

Sets or queries the stop offset frequency for plotting the phase noise trace.

Conditions Measurement views: Phase noise

Group Sense commands

Syntax `[SENSe]:PNOise:FREQuency:PLOT:OFFSet:STOP <value>`
`[SENSe]:PNOise:FREQuency:PLOT:OFFSet:STOP?`

Arguments `<value>::=<Nrf>` specifies the stop offset frequency for plot.
 It must be greater than the start offset frequency.
 Range: 100 Hz to 1 GHz in a tenfold sequence.

Examples `SENSE:PNOISE:FREQUENCY:PLOT:OFFSET:STOP 100MHz` sets the stop offset frequency for plot to 100 MHz.

[SENSe]:PNOise:OPTimization

Sets or queries the method of optimizing the gain and input bandwidth in the phase noise measurement.

Conditions Measurement views: Phase noise

Group Sense commands

Syntax `[SENSe]:PNOise:OPTimization { DRANge | SPEEd }`
`[SENSe]:PNOise:OPTimization?`

Arguments `DRANge` optimizes the gain and input bandwidth to maximize the dynamic range.
`SPEEd` optimizes the gain and input bandwidth to speed the measurement.

Examples SENSE:PNOISE:OPTIMIZATION DRANGE optimizes the gain and input bandwidth to maximize the dynamic range.

[SENSE]:POWER:UNITs

Sets or queries the fundamental unit of power.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:Power:UNITs { DBM | DBV | VOLTs | WATTs | DBUW | DBW | DBUV | DBMV | DBUA | DBUV_M | DBUA_M | AMPS }
[SENSE]:Power:UNITs?

Arguments The following table lists the arguments.

Table 2-43: Power units

Argument	Power unit
DBM	dBm
DBV	dBV
VOLTs	Volts
WATTs	Watts
DBUW	dB μ W
DBW	dBW
DBUV	dB μ V
DBMV	dBmV
DBUA	dB μ A
DBUV_M	dB μ V/m
DBUA_M	dB μ A/m
AMPS	Amps

NOTE. Select dB μ V/m or dB μ A/m unit when using an antenna table.

Examples SENSE:POWER:UNITs DBM specifies the fundamental unit of power as dBm.

[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:ALENgtH

Sets or queries the absolute amount of time included in the Frequency-Domain Linearity type measurements.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:ALENgtH <vaLue> [SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:ALENgtH?
Arguments	<vaLue>::=<Nrf> specifies the absolute time in seconds for the measurement time. Range: 1 ns to 100 seconds
Examples	[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:ALENgtH 1E-6 sets the measurement time to 1 μ s.

[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:MEthod

Sets or queries the measurement time method for the Frequency-Domain Linearity type measurements.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:MEthod { ABSolute RELative } [SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:MEthod?
Arguments	ABSolute specifies the absolute time in seconds based on rising edge of the pulse. RELative specifies the relative time in percent based on the pulse width and the center of the pulse.

Examples [SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:METHOD REL sets the time method to Relative.

[SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLENGTH

Sets or queries the relative amount of time included in the Frequency-Domain Linearity type measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLENGTH
<value>
[SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLENGTH?

Arguments <value>::=<Nrf> specifies the relative time in percent for the measurement time based on the pulse width and centered of the pulse.

Range: 10% to 100%

Examples [SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLENGTH 70 sets the measurement time to 70% of the pulse width.

[SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLEVEL

Sets or queries the measurement reference level for Frequency-Domain Linearity measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLEVEL
<value>
[SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLEVEL?

Arguments <value>::=<Nrf> specifies the reference level in percentage as the location on the voltage straight-line approximation of the pulse rising edge.

Range: 50% to 100%

Examples [SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:RLEVEL 60 sets the reference level to 60% of the rising edge.

[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:START

Sets or queries the start time for the Frequency-Domain Linearity type measurements. The start time is the amount of time wait after the rising-edge reference before starting to measure.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:START <value>
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:START?

Arguments <value>::=<Nrf> specifies the start time in seconds from the reference level of the rising edge of the pulse.

Range: -100 ms to 100 ms

Examples [SENSE]:PULSE:ANALYZE:FDOMAIN:MEASUREMENT:TIME:START 1E-6 sets the start time to 1 μ s.

[SENSe]:PULSe:ANALyze:IRESponse:CORRection:AMPLitude[:STATe]

Enables or disables the corrections for window and for delay of the highest side lobe in the Pulse Impulse Response measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:ANALyze:IRESponse:CORRection:AMPLitude[:STATe]
{ OFF | ON | 0 | 1 }
[SENSe]:PULSe:ANALyze:IRESponse:CORRection:AMPLitude[:
STATe]?

Arguments OFF or 0 disables amplitude correction in Impulse Response measurements.
ON or 1 enables amplitude correction in Impulse Response measurements.

Examples [SENSE]:PULSE:ANALYZE:IRESPONSE:CORRECTION:AMPLITUDE[:STATE]
1 enables amplitude correction.

[SENSE]:PULSE:ANALYZE:IRESPONSE:KOTIME

Sets or queries the Keep-out time in the Pulse Impulse Response measurements. This specifies the width of time around the main lobe that lobes within this time zone are not eligible to be the “highest side lobe.”

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSE]:PULSE:ANALYZE:IRESPONSE:KOTIME <value>
[SENSE]:PULSE:ANALYZE:IRESPONSE:KOTIME?

Arguments <value>::=<NRF> specifies the Keep-out time in seconds.
Range: 0 to 100 seconds.

Examples [SENSE]:PULSE:ANALYZE:IRESPONSE:KOTIME 0.001 sets the keep-out time to 1 ms.

[SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:ALENGTH

Sets or queries the absolute amount of time included in the Impulse Response type measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:ALENGTH
<value>
[SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:ALENGTH?

Arguments <value>::=<Nrf> specifies the absolute time in seconds for the measurement time.

Range: 1 ns to 100 seconds.

Examples [SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:ALENGTH 1E-6 sets the measurement time to 1 μ s.

[SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:METHOD

Sets or queries the measurement time method for the Impulse Response type measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:METHOD { ABSolute | RELative }
[SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:METHOD?

Arguments ABSolute specifies the absolute time in seconds based on rising edge of the pulse.
RELative specifies the relative time in percent based on the pulse width and the center of the pulse.

Examples [SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:METHOD REL sets the time method to Relative.

[SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:RELEngth

Sets or queries the relative amount of time included in the Impulse Response type measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:RELEngth <value>

[SENSE]:PULSE:ANALyze:IRESpOse:MEASurement:TIME:RLEnGth?

Arguments <value>::=<NRf> specifies the relative time in percent for the measurement time based on the pulse width and centered of the pulse.

Range: 10% to 100%.

Examples [SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:RLENGTH 70 sets the measurement time to 70% of the pulse width.

[SENSE]:PULSE:ANALyze:IRESpOse:MEASurement:TIME:RLEVel

Sets or queries the measurement reference level for Impulse Response measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSE]:PULSE:ANALyze:IRESpOse:MEASurement:TIME:RLEVel
<value>
[SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:RLEVEL?

Arguments <value>::=<NRf> specifies the reference level in percentage as the location on the voltage straight-line approximation of the pulse rising edge.

Range: 50% to 100%.

Examples [SENSE]:PULSE:ANALYZE:IRESPONSE:MEASUREMENT:TIME:RLEVEL 60 sets the reference level to 60% of the rising edge.

[SENSE]:PULSE:ANALyze:IRESpOse:MEASurement:TIME:STARt

Sets or queries the start time for the Impulse Response type measurements. The start time is the amount of time wait after the rising-edge reference before starting to measure.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:START
 <value>
 [SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:START?

Arguments <value>::=<NRF> specifies the start time in seconds from the reference level of the rising edge of the pulse.
 Range: -100 ms to 100 ms.

Examples [SENSe]:PULSe:ANALyze:IRESponse:MEASurement:TIME:START 1E-6
 sets the start time to 1 μ s.

[SENSe]:PULSe:ANALyze:LEVel

Sets or queries how to determine the 50% level for the pulsed RF measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:ANALyze:LEVel { VOLTage | POWER }
 [SENSe]:PULSe:ANALyze:LEVel?

Arguments VOLTage uses -6 dB to determine the 50% level.
 POWER uses -3 dB to determine the 50% level.

Examples SENSE:PULSe:ANALyze:LEVel POWER sets RF measurements to use -3 dB to determine the 50% level.

[SENSe]:PULSe:ANALyze:LEVel:FIFTy

Sets or queries how to determine the 50% level for the pulsed RF measurements. This command is equivalent to the [\[SENSe\]:PULSe:ANALyze:LEVel](#) command.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax	<code>[SENSe]:PULSe:ANALyze:LEVe] :FIFTy { VOLTage POWer } [SENSe]:PULSe:ANALyze:LEVe] :FIFTy?</code>
Arguments	<code>VOLTage</code> uses -6 dB to determine the 50% level. <code>POWer</code> uses -3 dB to determine the 50% level.
Examples	<code>SENSe:PULSe:ANALyze:LEVe] :FIFTy POWer</code> sets RF measurements to use -3 dB to determine the 50% level.

[SENSe]:PULSe:ANALyze:LEVe] :HUNDred

Sets or queries how to determine the 100% level in the pulsed RF measurements. This command is equivalent to the [\[SENSe\]:PULSe:ANALyze:POINT:LOCation](#) command.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	<code>[SENSe]:PULSe:ANALyze:LEVe] :HUNDred { AVERage INDepe]ndent } [SENSe]:PULSe:ANALyze:LEVe] :HUNDred?</code>

Related Commands

Arguments	<code>AVERage</code> uses the average amplitude calculated for the pulse-on as the 100% reference to measure the rise and fall times. <code>INDepe]ndent</code> uses the amplitudes at the beginning and end of the pulse-on as the 100% references to measure the rise and fall times, respectively
Examples	<code>SENSe:PULSe:ANALyze:LEVe] :HUNDred AVERage</code> uses pulse average amplitude to set the 100% level.

[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:ALEN]gth

Sets or queries the absolute amount of time included in the Overshoot measurements.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
-------------------	---

Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:ALENgtH <vaLue> [SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:ALENgtH?
Arguments	<vaLue> ::= <NRf> specifies the absolute time in seconds for the measurement time. Range: 1 ns to 100 seconds
Examples	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:ALENgtH 1E-6 sets the measurement time to 1 μ s.

[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:MEtHod

Sets or queries the measurement time method for the Overshoot measurements.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:MEtHod { ABSolute RELative } [SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:MEtHod?
Arguments	ABSolute specifies the absolute time in seconds based on rising edge of the pulse. RELative specifies the relative time in percent based on the pulse width and the center of the pulse.
Examples	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:MEtHod REL sets Overshoot measurements to use the relative time method.

[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RELEngtH

Sets or queries the relative amount of time included in the Overshoot measurements.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
-------------------	---

Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEnGth <value> [SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEnGth?
Arguments	<value>::=<NRf> specifies the relative time in percent for the measurement time based on the pulse width and centered of the pulse. Range: 0.01% to 100%.
Examples	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEnGth 70 sets the measurement time to 70% of the pulse width.

[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEVel

Sets or queries the measurement reference level for the Overshoot measurements.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEVel <value> [SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEVel?
Arguments	<value>::=<NRf> specifies the reference level in percentage as the location on the voltage straight-line approximation of the pulse rising edge. Range: 50% to 100%.
Examples	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEVel 60 sets the reference level to 60% of the rising edge.

[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:STARt

Sets or queries the start time for the Overshoot measurements. The start time is the amount of time wait after the rising-edge reference before starting to measure.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
-------------------	---

Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:START <value> [SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:START?
Arguments	<value> ::= <NRF> specifies the start time in seconds from the reference level of the rising edge of the pulse. Range: -100 ms to 100 ms.
Examples	[SENSe]:PULSe:ANALyze:OVERSHOOT:MEASUREMENT:TIME:START 1E-6 sets the start time to 1 μ s.

[SENSe]:PULSe:ANALyze:PMLocation

Sets or queries the phase measurement location (the position along the pulse tops where the phase is measured) in the pulse-pulse phase measurement.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	[SENSe]:PULSe:ANALyze:PMLocation <value> [SENSe]:PULSe:ANALyze:PMLocation?
Arguments	<value> ::= <NRF> specifies the pulse-pulse phase measurement location. Range: 5 ns to 100 ms.
Examples	SENSE:PULSE:ANALYZE:PMLOCATION 1.5ms sets the phase measurement location to 1.5 ms.

[SENSe]:PULSe:ANALyze:POINT:LOCation

Sets or queries the point location method in the pulsed RF measurements.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands

Syntax	<code>[SENSe]:PULSe:ANALyze:POINt:LOCation { AVERAge INDePendent } [SENSe]:PULSe:ANALyze:POINt:LOCation?</code>
Arguments	<code>AVERAge</code> uses the average amplitude calculated for the pulse-on as the 100% reference to measure the rise and fall times. <code>INDePendent</code> uses the amplitudes at the beginning and end of the pulse-on as the 100% references to measure the rise and fall times, respectively.
Examples	<code>SENSE:PULSE:ANALYZE:POINT:LOCATION AVERAge</code> uses pulse average amplitude to locate points.

[SENSe]:PULSe:ANALyze:RFALl

Sets or queries the threshold levels to measure the rise/fall time.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	<code>[SENSe]:PULSe:ANALyze:RFALl { WIDE NARROW } [SENSe]:PULSe:ANALyze:RFALl?</code>
Arguments	<code>WIDE</code> selects 10 - 90% to measure the rise/fall time. <code>NARROW</code> selects 20 - 80% to measure the rise/fall time.
Examples	<code>SENSE:PULSE:ANALYZE:RFALL WIDE</code> selects 10 - 90% to measure the rise/fall time.

[SENSe]:PULSe:ANALyze:RIPPlE

Sets or queries the ripple portion of the pulse top (how much of the beginning and end of the pulse top to exclude from the ripple calculation).

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands

Syntax [SENSE]:PULSE:ANALyze:RIPPlE <value>
[SENSE]:PULSE:ANALyze:RIPPlE?

Arguments <value>::=<NRF> specifies the ripple portion of the pulse top.
Range: 10 to 100% in 1% steps.

Examples SENSE:PULSE:ANALYZE:RIPPLE 30 sets the ripple portion to 30% of the pulse top.

[SENSE]:PULSE:CARRIER:FREQUENCY? (Query Only)

Queries the carrier frequency.

Conditions Measurement views: Pulse table

Group Sense commands

Syntax [SENSE]:PULSE:CARRIER:FREQUENCY?

Related Commands [\[SENSE\]:PULSE:CARRIER:OFFSET](#)

Arguments None

Returns <NRF> indicates the actual carrier frequency in Hz.

Examples SENSE:PULSE:CARRIER:FREQUENCY? might return 2.7000001690E+9, indicating that the pulse carrier frequency is 2.700000169 GHz.

[SENSE]:PULSE:CARRIER:OFFSET

Sets or queries the carrier frequency offset.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSE]:PULSE:CARRIER:OFFSET <value>
[SENSE]:PULSE:CARRIER:OFFSET?

Related Commands [\[SENSE\]:PULSE:CARRIER:SEARCH](#)

Arguments <value> ::= <NRF> specifies the carrier frequency offset.
Range: -50 kHz to +50 kHz.

Examples SENSE:PULSE:CARRIER:OFFSET 2.5kHz sets the offset frequency to 2.5 kHz to the carrier.

[SENSE]:PULSE:CARRIER:SEARCH

Sets or queries how to detect the carrier in the pulsed RF measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSE]:PULSE:CARRIER:SEARCH { AUTO | MANUAL }
[SENSE]:PULSE:CARRIER:SEARCH?

Arguments AUTO specifies that the carrier is detected automatically.
MANUAL specifies that the carrier frequency offset is set manually, using the [\[SENSE\]:PULSE:CARRIER:OFFSET](#) command.

Examples SENSE:PULSE:CARRIER:SEARCH AUTO specifies that the carrier is detected automatically.

[SENSE]:PULSE:DETECT:MEASUREMENT

Determines whether or not to set the maximum number of pulses to measure within the analysis time.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:DETEct:MEASurement { OFF | ON | 0 | 1 }
[SENSe]:PULSe:DETEct:MEASurement?

Arguments OFF or 0 measures all pulses (max. 1000) in the analysis time.
ON or 1 specifies that the maximum number of pulses is set manually, using the [SENSe]:PULSe:DETEct:NUMBer command.

Examples SENSE:PULSE:DETECT:MEASUREMENT ON specifies that the maximum number of pulses is set manually.

[SENSe]:PULSe:DETEct:NUMBer

Sets or queries the maximum number of pulses to measure within the analysis time when [SENSe]:PULSe:DETEct:MEASurement is On.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:DETEct:NUMBer <value>
[SENSe]:PULSe:DETEct:NUMBer?

Arguments <value>::=<NRF> specifies the maximum number of pulses to measure within the analysis time. Range: 1 to 1000.
If the analysis time contains fewer pulses than this number, all of these are measured.

Examples SENSE:PULSE:DETECT:NUMBER 850 sets the maximum number of pulses to 850.

[SENSe]:PULSe:DETEct:POWer[:THReshold]

Sets or queries the power threshold to detect pulses.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax	<code>[SENSE]:PULSE:DETECT:POWER[:THRESHOLD] <value></code> <code>[SENSE]:PULSE:DETECT:POWER[:THRESHOLD]?</code>
Arguments	<code><value> ::= <NRF></code> specifies the power threshold to detect pulses. Range: -70 to 0 dB.
Examples	<code>SENSE:PULSE:DETECT:POWER:THRESHOLD -20</code> sets the power threshold to -20 dB.

[SENSE]:PULSE:DETECT:TIME[:THRESHOLD]

Sets or queries the minimum off-time between pulses.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	<code>[SENSE]:PULSE:DETECT:TIME[:THRESHOLD] <value></code> <code>[SENSE]:PULSE:DETECT:TIME[:THRESHOLD]?</code>
Arguments	<code><value> ::= <NRF></code> specifies the minimum off-time between pulses. Range: 1 ns to 100 ms.
Examples	<code>SENSE:PULSE:DETECT:TIME:THRESHOLD 1.5ms</code> sets the time threshold to 1.5 ms.

[SENSE]:PULSE:FILTER:{BANDWIDTH|BWIDTh}

Sets or queries the filter or acquisition bandwidth when `[SENSE]:PULSE:FILTER:MEASUREMENT` is set to GAUSSian or NONE (No filter), respectively.

Conditions	Measurement views: Pulse statistics, Pulse table, Pulse trace
Group	Sense commands
Syntax	<code>[SENSE]:PULSE:FILTER:{BANDWIDTH BWIDTh} <value></code> <code>[SENSE]:PULSE:FILTER:{BANDWIDTH BWIDTh}?</code>

Related Commands [\[SENSe\]:PULSe:FILTer:MEASurement](#)

Arguments `<value> ::= <NRF>` specifies the filter/acquisition bandwidth depending the [SENSe]:PULSe:FILTer:MEASurement setting. The table below shows the setting range. You can enter any value, but it is rounded up to the next valid number.

[SENSe]:PULSe:FILTer:MEASurement	Range
GAUSSian	100 Hz to 20 MHz (Standard) / 100 Hz to 55 MHz (Option 110) in 1-2-3-5 sequence.
NONE	152, 305, 610, 1.22 k, 2.44 k, 4.88 k, 9.76 k, 19.3 k, 39 k, 78 k, 156 k, 312 k, 625 k, 1.25 M, 2.5 M, 5 M, 10 M, 20 M, 40 MHz, and optionally 60 M and 110 MHz (Option 110).

Examples `SENSE:PULSE:FILTER:BANDWIDTH 10MHZ` sets the filter bandwidth to 10 MHz.

[SENSe]:PULSe:FILTer:MEASurement

Sets or queries the measurement filter in the pulsed RF measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax `[SENSe]:PULSe:FILTer:MEASurement { GAUSSian | NONE | MAXRtbw }`
`[SENSe]:PULSe:FILTer:MEASurement?`

Related Commands [\[SENSe\]:PULSe:FILTer:{BANDwidth|BWIDth}](#)

Arguments `GAUSSian` uses the Gaussian filter in the pulsed RF measurements. Use the `[SENSe]:PULSe:FILTer:{BANDwidth|BWIDth}` command to set the filter bandwidth.

`NONE` uses no filter. Use the `[SENSe]:PULSe:FILTer:{BANDwidth|BWIDth}` command to set the acquisition bandwidth.

`MAXRtbw` uses no filter. The acquisition bandwidth is fixed to the maximum real-time bandwidth: 40 MHz (Standard) or 110 MHz (Option 110).

Examples `SENSE:PULSE:FILTER:MEASUREMENT GAUSSian` uses the Gaussian filter in the pulsed RF measurements.

[SENSe]:PULSe:FREFerence:AUTO

Determines whether to estimate the pulse frequency reference automatically or manually in the pulsed RF measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax `[SENSe]:PULSe:FREFerence:AUTO { OFF | ON | 0 | 1 }`
`[SENSe]:PULSe:FREFerence:AUTO?`

Arguments OFF or 0 estimates the frequency reference manually. Use the [\[SENSe\]:PULSe:FREFerence:OFFSet](#) command to set the frequency offset.
 ON or 1 estimates the frequency reference automatically.

Examples `SENSE:PULSE:FREFERENCE:AUTO ON` specifies that the frequency reference is estimated automatically.

[SENSe]:PULSe:FREFerence:CSLope

Sets or queries the Chirp Slope.

Chirp Slope is used when the Modulation Type is set to Linear Chirp. When set, this also changes the Chirp Slope to manual mode. When chirp slope is in auto mode, the query returns the estimated chirp slope.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax `[SENSe]:PULSe:FREFerence:CSLope <value>`
`[SENSe]:PULSe:FREFerence:CSLope?`

Arguments <value>:=NRF specifies the chirp slope in Hz/μs.

Range: -100 GHz/μs to 100 GHz/μs.

Examples [SENSE]:PULSE:FREFERENCE:CSLOPE 1E6 sets the chirp slope to 1 MHz/μs.

[SENSe]:PULSe:FREference:CSLoPe:AUTO

Sets or queries enabling automatic Chirp Slope estimating in the pulsed RF measurements.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:FREference:CSLoPe:AUTO { OFF | ON | 0 | 1 }
[SENSe]:PULSe:FREference:CSLoPe:AUTO?

Arguments OFF or 0 estimates the chirp slope manually. Use the [SENSe]:PULSe:FREFERENCE:CSLOPE command to set the chirp slope.

ON or 1 estimates the chirp slope automatically.

Examples [SENSE]:PULSE:FREFERENCE:CSLOPE:AUTO 1 sets the chirp slope to auto mode.

[SENSe]:PULSe:FREference:OFFSet

Sets or queries the frequency reference offset. This command is valid when [SENSe]:PULSe:FREFERENCE:AUTO is set to OFF.

Conditions Measurement views: Pulse statistics, Pulse table, Pulse trace

Group Sense commands

Syntax [SENSe]:PULSe:FREference:OFFSet <value>
[SENSe]:PULSe:FREference:OFFSet?

- Arguments** `<value> ::= <Nrf>` specifies the frequency reference offset.
Range: -50 kHz to +50 kHz.
- Examples** `SENSE:PULSE:REFERENCE:OFFSET 2.5kHz` sets the frequency offset to 2.5 kHz to the reference.

[SENSe]:PULSe:MODulation:TYPE

Sets or queries the modulation type in the pulsed RF measurements. This command is equivalent to the [\[SENSe\]:REANalyze:NEXT](#) command.

- Conditions** Measurement views: Pulse statistics, Pulse table, Pulse trace
- Group** Sense commands
- Syntax** `[SENSe]:PULSe:MODulation:TYPE { CWConst | CWCHange | LCHirp | OTHER }`
`[SENSe]:PULSe:MODulation:TYPE?`
- Arguments** `CWConst` selects the CW (continuous wave) with constant phase.
`CWCHange` selects the CW (continuous wave) with changing phase.
`LCHirp` selects the linear chirp.
`OTHER` selects other.
- Examples** `SENSE:PULSE:MODULATION:TYPE CWCHange` selects the CW with changing phase as the modulation type.

[SENSe]:PULSe:SIGNal:TYPE

Sets or queries the signal type in the pulsed RF measurements.

- Conditions** Measurement views: Pulse statistics, Pulse table, Pulse trace
- Group** Sense commands
- Syntax** `[SENSe]:PULSe:SIGNal:TYPE { CWConst | CWCHange | LCHirp | OTHER }`

[SENSE]:PULSE:SIGNAL:TYPE?

- Arguments** CWConst selects CW (continuous wave) with constant phase.
 CWCHange selects CW (continuous wave) with changing phase.
 LCHi rp selects linear chirp.
 OTHER selects other.
- Examples** SENSE:PULSE:SIGNAL:TYPE CWCHange selects the CW with changing phase as the signal type.

[SENSE]:PULSE:STATistics:HISTogram:ORDinate

Sets or queries the Histogram Y unit. This command is valid when [DISPlay:PULSE:STATistics:PLOT](#) is set to Histogram.

- Conditions** Measurement views: Pulse statistics
- Group** Sense commands
- Syntax** [SENSE]:PULSE:STATistics:HISTogram:ORDinate { PERCent | COUNT }
 [SENSE]:PULSE:STATistics:HISTogram:ORDinate?
- Arguments** PERCent sets the Histogram plot Y axis to the percentage of points.
 COUNT sets the Histogram plot Y axis to the number of points in the bin.
- Examples** [SENSE]:PULSE:STATISTICS:HISTOGRAM:ORDINATE PERCENT sets the histogram Y axis to percent.

[SENSE]:PULSE:STATistics:HISTogram:POINTS

Sets or queries the number of bins in the Histogram plot.

- Conditions** Measurement views: Pulse statistics
- Group** Sense commands

Syntax	[SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS <value> [SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS?
Arguments	<value>::=<NRF> specifies the number of histogram bins. Range: 5 to 10000
Examples	[SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS 10 sets the number of histogram bins to 10.

[SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS:AUTO

Sets or queries enabling automatic Histogram plot bins count.

Conditions	Measurement views: Pulse statistics
Group	Sense commands
Syntax	[SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS:AUTO { OFF ON 0 1 } [SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS:AUTO?
Arguments	OFF or 0 sets the number of bins manually by the [SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS command. ON or 1 sets the number of bins to the number of pulses/10.
Examples	[SENSE]:PULSE:STATISTICS:HISTOGRAM:POINTS:AUTO 1 sets the number of histogram bins based on number of pulses.

[SENSE]:REANalyze (No Query Form)

Sets all measurements to reanalyze the last acquisition.

NOTE. *SENSE:REANalyze is an overlapped command, which does not finish executing before the next command starts executing. Use the *OPC(?) and *WAI commands to synchronize all pending operations to the execution of this command.*

Conditions	Measurement views: All
-------------------	------------------------

Group	Sense commands
Syntax	[SENSE]:REANalyze
Related Commands	*OPC, *WAI
Arguments	None
Examples	SENSE:REANALYZE reanalyzes all measurements using the current acquisition.

[SENSE]:REANalyze:ACQuisition:SETTings? (Query Only)

Queries the settings of all acquisitions.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSE]:REANalyze:ACQuisition:SETTings?

[SENSE]:REANalyze:ALL (No Query Form)

Replay all items in the current acquisition selection.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSE]:REANalyze:ALL

[SENSE]:REANalyze:CURRent (No Query Form)

Replay the currently selected acquisition (or frame).

Conditions	Measurement views: All
-------------------	------------------------

Group Sense commands

Syntax [SENSE]:REANalyze:CURRENT

[SENSE]:REANalyze:CURRENT:ACQuisition? (Query Only)

Queries the Acquisition record identifier (ID) of the currently selected acquisition (or frame).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:CURRENT:ACQuisition?

[SENSE]:REANalyze:CURRENT:FRAME? (Query Only)

Queries the Frame identifier (ID) of the currently selected acquisition (or frame).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:CURRENT:FRAME?

[SENSE]:REANalyze:CURRENT:TIMEstamp? (Query Only)

Queries the timestamp of the currently selected acquisition (or frame).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:CURRENT:TIMEstamp?

[SENSe]:REANalyze:DELeTe:DATA (No Query Form)

Deletes all acquisition data.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:DELeTe:DATA

[SENSe]:REANalyze:FIRSt (No Query Form)

Replays (reanalyzes) the first item in the currently selected acquisition (or frame).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:FIRSt

[SENSe]:REANalyze:LAST (No Query Form)

Replays (reanalyzes) the last item in the currently selected acquisition (or frame).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:LAST

[SENSe]:REANalyze:NEXt (No Query Form)

Replays (reanalyzes) the next item in the currently selected acquisition (or frame).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:NEXT

[SENSE]:REANalyze:PAUSE

Sets or queries the reanalysis paused state.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:PAUSE {OFF | ON | 0 | 1 }
[SENSE]:REANalyze:PAUSE?

Arguments ON or 1 pauses (blocks) any acquisition until current reanalysis is completed.
OFF or 0 disables the reanalysis pause mode.

[SENSE]:REANalyze:PREVIOUS (No Query Form)

Replays (reanalyzes) the previous item in the currently selected acquisition (or frame).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:PREVIOUS

[SENSE]:REANalyze:SElect:ACquisition:FIRSt? (Query Only)

Queries the first selectable acquisition Start or Stop value in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:SElect:ACQuisition:FIRSt?

Related Commands [\[SENSe\]:REANalyze:SElect:ACQuisition:FIRSt:TIMestamp?](#)

[SENSe]:REANalyze:SElect:ACQuisition:FIRSt:TIMestamp? (Query Only)

Queries the timestamp of the first selectable acquisition history Start or Stop value in the currently selected acquisition set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:ACQuisition:FIRSt:TIMestamp?

Related Commands [\[SENSe\]:REANalyze:SElect:ACQuisition:FIRSt?](#)

[SENSe]:REANalyze:SElect:ACQuisition:LAST? (Query Only)

Queries the last selectable acquisition Start or Stop value in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:ACQuisition:LAST?

Related Commands [\[SENSe\]:REANalyze:SElect:ACQuisition:LAST:TIMestamp?](#)

[SENSe]:REANalyze:SElect:ACQuisition:LAST:TIMestamp? (Query Only)

Queries the timestamp of the last selectable acquisition Start or Stop value in the currently selected set.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSE]:REANalyze:SElect:ACQuisition:LAST:TIMestamp?
Related Commands	[SENSe]:REANalyze:SElect:ACQuisition:LAST?

[SENSE]:REANalyze:SElect:ACQuisition:START

Sets or queries the Acquisition Start value in the currently selected set.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSE]:REANalyze:SElect:ACQuisition:START <value> [SENSe]:REANalyze:SElect:ACQuisition:START?
Arguments	<value> ::= <NR1> is an integer in the range from one to the number of acquisitions in the acquisition history.

[SENSe]:REANalyze:SElect:ACQuisition:START:TIMestamp? (Query Only)

Queries the timestamp of the current Acquisition Start selection. It is the timestamp of the first frame of the selected acquisition, if FastFrame is enabled.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:REANalyze:SElect:ACQuisition:START:TIMestamp?

[SENSE]:REANalyze:SElect:ACQuisition:STOP

Sets or queries the Acquisition Stop value in the currently selected set.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSE]:REANalyze:SElect:ACQuisition:STOP <value> [SENSE]:REANalyze:SElect:ACQuisition:STOP?
Arguments	<value>::=<NR1> is an integer in the range from one to the number of acquisitions in the acquisition history.

[SENSE]:REANalyze:SElect:ACQuisition:STOP:TIMestamp? (Query Only)

Queries the timestamp of the current Acquisition Stop selection. This is the Timestamp of the last frame of the selected acquisition, if FastFrame is enabled.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSE]:REANalyze:SElect:ACQuisition:STOP:TIMestamp?

[SENSE]:REANalyze:SElect:ALL (No Query Form)

Selects all acquisitions and frames in the currently selected set.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSE]:REANalyze:SElect:ALL

[SENSE]:REANalyze:SElect:FRAMe:FIRSt? (Query Only)

Queries the first available Frame Start or Stop value available in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:FIRSt?

Related Commands [\[SENSe\]:REANalyze:SElect:FRAMe:FIRSt:TIMestamp?](#)

[SENSe]:REANalyze:SElect:FRAMe:FIRSt:TIMestamp? (Query Only)

Queries the timestamp of the first available frame of the first available Acquisition Start or Stop value available in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:FIRSt:TIMestamp?

Related Commands [\[SENSe\]:REANalyze:SElect:FRAMe:FIRSt?](#)

[SENSe]:REANalyze:SElect:FRAMe:LAST? (Query Only)

Queries the last available Frame Start or Stop value available in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:LAST?

Related Commands [\[SENSe\]:REANalyze:SElect:FRAMe:LAST:TIMestamp?](#)

[SENSe]:REANalyze:SElect:FRAMe:LAST:TIMestamp? (Query Only)

Queries the timestamp of the last available frame of the last available Acquisition Start or Stop value available in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:LAST:TIMestamp?

Related Commands [\[SENSe\]:REANalyze:SElect:FRAMe:LAST?](#)

[SENSe]:REANalyze:SElect:FRAMe:START

Sets or queries the Frame Start value in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:START <value>
[SENSe]:REANalyze:SElect:FRAMe:START?

Arguments <value>::=<NR1> is an integer in the range from one to the number of fast frames.

[SENSe]:REANalyze:SElect:FRAMe:START:TIMestamp? (Query Only)

Queries the timestamp of the current Frame Start selection. This is the timestamp of the Frame Start frame of the acquisition start acquisition, if FastFrame is enabled.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:START:TIMestamp?

[SENSe]:REANalyze:SElect:FRAMe:STOP

Sets or queries the frame stop value in the currently selected set.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:STOP <value>
[SENSe]:REANalyze:SElect:FRAMe:STOP?

Related Commands [\[SENSe\]:REANalyze:SElect:FRAMe:STOP:TIMestamp?](#)

Arguments <value> ::= <NR1> is an integer in the range from one to the number of fast frames.

[SENSe]:REANalyze:SElect:FRAMe:STOP:TIMestamp? (Query Only)

Queries the timestamp of the current frame stop selection. It is the timestamp of the frame Stop frame of the Acquisition Stop acquisition, if FastFrame is enabled

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:REANalyze:SElect:FRAMe:STOP:TIMestamp?

Related Commands [\[SENSe\]:REANalyze:SElect:FRAMe:STOP](#)

[SENSe]:REANalyze:SPEed

Sets or queries the time delay value inserted between reanalysis of frames or acquisitions.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:SPEEd <value>
[SENSE]:REANalyze:SPEEd?

Arguments <value>::=<NR1> is an integer in the range of zero (for no delay) to four (for a maximum delay of about one second).

[SENSE]:REANalyze:STOP (No Query Form)

Stops the current reanalysis. The command will block until the current reanalysis has completed and stopped.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:STOP

[SENSE]:REANalyze:TIMestamp:DECimal

Sets or queries the number of values to the right of the decimal point to include in all timestamps.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSE]:REANalyze:TIMestamp:DECimal <value>
[SENSE]:REANalyze:TIMestamp:DECimal?

Arguments <value>::=<NR1> is an integer in the range of one to nine.

[SENSE]:ROSCillator:SOURce

Sets or queries the frequency reference oscillator source.

Conditions	Measurement views: All
Group	Sense commands
Syntax	<code>[SENSe]:ROSCillator:SOURCE { INTERNAL EXTERNAL }</code> <code>[SENSe]:ROSCillator:SOURCE?</code>
Arguments	<p><code>INTERNAL</code> specifies that the analyzer uses the 10 MHz internal oscillator.</p> <p><code>EXTERNAL</code> specifies that the analyzer uses the external reference signal. Use the Ref In connector on the rear panel to input the signal.</p> <p>Selecting <code>EXTERNAL</code> initiates an attempt to lock the internal reference oscillator to the external reference signal. If the signal is not connected or is at an invalid frequency or amplitude, an error (2028, "External frequency reference signal not valid. Using internal reference") is returned. If not able to lock to the external reference, an error (2029, "Unable to lock to external frequency reference. Using internal reference.") is returned.</p>
Examples	<code>SENSE:ROSCILLATOR:SOURCE INTERNAL</code> uses the 10 MHz internal oscillator for the frequency reference.

[SENSe]:SGRam:{BANDwidth|BWIDth}:OPTimization

Sets or queries the method of optimizing the gain and input bandwidth in the spectrogram.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	<code>[SENSe]:SGRam:{BANDwidth BWIDth}:OPTimization { AUTO MAXDynrange MINNoise MINTime }</code> <code>[SENSe]:SGRam:{BANDwidth BWIDth}:OPTimization?</code>
Arguments	<p><code>AUTO</code> optimizes automatically the gain and input bandwidth.</p> <p><code>MAXDynrange</code> optimizes the gain and input bandwidth to maximize the dynamic range.</p> <p><code>MINNoise</code> optimizes the gain and input bandwidth to minimize noise.</p> <p><code>MINTime</code> optimizes the gain and input bandwidth to minimize sweep time.</p>

Examples `SENSE:SGRAM:BANDWIDTH:OPTIMIZATION AUTO` optimizes automatically the gain and input bandwidth.

[SENSe]:SGRam:{BANDwidth|BWIDth}:RESolution

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets `[SENSe]:SGRam{BANDwidth|BWIDth}:RESolution:AUTO OFF`.

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax `[SENSe]:SGRam:{BANDwidth|BWIDth}:RESolution <value>`
`[SENSe]:SGRam:{BANDwidth|BWIDth}:RESolution?`

Related Commands [\[SENSe\]:SGRam:{BANDwidth|BWIDth}\[:RESolution\]:AUTO](#)

Arguments `<value>::=<NRF>` specifies the RBW. Range: 1 Hz to 10 MHz.

Examples `SENSE:SGRAM:BANDWIDTH:RESOLUTION 200kHz` sets the RBW to 200 kHz.

[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the spectrogram.

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax `[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:ACTual?`

Arguments None

Returns `<NRF>` The actual RBW in Hz.

Examples `SENSE:SGRAM:BANDWIDTH:RESOLUTION:ACTUAL?` might return `299.624E+3`, indicating that the actual RBW is 299.624 kHz.

`[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:AUTO`

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the spectrogram.

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax `[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:AUTO { OFF | ON | 0 | 1 }`
`[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:AUTO?`

Arguments OFF or 0 specifies that the resolution bandwidth is set manually using the `[SENSe]:DPSA:{BANDwidth|BWIDth}:ACTual?` command.
 ON or 1 specifies that the resolution bandwidth is set automatically.

Examples `SENSE:SGRAM:BANDWIDTH:RESOLUTION:AUTO ON` sets the resolution bandwidth automatically.

`[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:MODE`

Determines whether to enable or disable the RBW processing in the spectrogram.

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax `[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:MODE { OFF | ON | 0 | 1 }`
`[SENSe]:SGRam:{BANDwidth|BWIDth}[:RESolution]:MODE?`

Arguments OFF or 0 disables the RBW processing. You can select the FFT window using the `[SENSe]:SGRam:FFT:WINDow` command.

ON or 1 enables the RBW processing. Refer to the [\[SENSe\]:SGRam:{BANDwidth|BWIDth}:RESolution](#) command to set the RBW.

Examples SENSE:SGRAM:BANDWIDTH:RESOLUTION:MODE ON enables the RBW processing.

[SENSe]:SGRam:{BANDwidth|BWIDth}:VIDeo

Sets or queries the video bandwidth (VBW). Programming a specified VBW sets [SENSe]:SGRam:{BANDwidth|BWIDth}:VIDeo:STATe OFF.

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax [SENSe]:SGRam:{BANDwidth|BWIDth}:VIDeo <value>
[SENSe]:SGRam:{BANDwidth|BWIDth}:VIDeo?

Related Commands [\[SENSe\]:SGRam:{BANDwidth|BWIDth}:VIDeo:STATe](#)

Arguments <value>::=<nrf> specifies the VBW.
Range: Current RBW/10⁴ (1 Hz minimum) to Current RBW.

Examples SENSE:SGRAM:BANDWIDTH:VIDEO 200kHz sets the VBW to 200 kHz.

[SENSe]:SGRam:{BANDwidth|BWIDth}:VIDeo:STATe

Determines whether to enable or disable the video bandwidth (VBW) in the spectrogram measurement.

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax [SENSe]:SGRam:{BANDwidth|BWIDth}:VIDeo:STATe { OFF | ON | 0 | 1 }
[SENSe]:SGRam:{BANDwidth|BWIDth}:VIDeo:STATe?

Arguments OFF or 0 disables the VBW.
ON or 1 enables the VBW.

Examples SENSE:SGRAM:BANDWIDTH:VIDEO:STATE ON enables the VBW.

[SENSe]:SGRam:COLor

Sets or queries the color palette of three-dimensional graphs.

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax [SENSe]:SGRam:COLor { RED | GREen | BLUe | CYAN | BCYan |
YELLow | MAGenta | GRAY | TEMPerature | SPECTral }
[SENSe]:SGRam:COLor?

Arguments The following table lists the arguments.

Table 2-44: Color palette for spectrogram

Argument	Palette
RED	Red
GREen	Green
BLUe	Blue
CYAN	Cyan
BCYan	Binary cyan
YELLow	Yellow
MAGenta	Magenta
GRAY	Gray
TEMPerature	Temperature
SPECTral	Spectral

Examples SENSE:SGRAM:COLOR TEMPerature selects the temperature color palette.

[SENSe]:SGRam:COLor:MAXimum

Sets or queries the maximum value of the color axis in the spectrogram.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSE]:SGRAM:COLOR:MAXimum <value> [SENSE]:SGRAM:COLOR:MAXimum?
Related Commands	[SENSe]:SGRAM:COLor:MINimum
Arguments	<value>::=<Nrf> specifies the maximum value of the color axis. Range: -100 to +100 dBm.
Examples	SENSE:SGRAM:COLOR:MAXIMUM 10 sets the maximum value of the color axis to 10 dBm.

[SENSe]:SGRAM:COLor:MINimum

Sets or queries the minimum value of the color axis in the spectrogram.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSe]:SGRAM:COLor:MINimum <value> [SENSe]:SGRAM:COLor:MINimum?
Related Commands	[SENSe]:SGRAM:COLor:MAXimum
Arguments	<value>::=<Nrf> specifies the minimum value of the color axis. Range: -100 to +100 dBm.
Examples	SENSE:SGRAM:COLOR:MINIMUM 10 sets the minimum value of the color axis to 10 dBm.

[SENSe]:SGRam:FFT:WINDow

Sets or queries the FFT window in the spectrogram. This command is equivalent to [\[SENSe\]:SGRam:FILTer\[:SHAPE\]](#).

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSe]:SGRam:FFT:WINDow { KAISer MIL6db CISPr BH4B UNIFORM FLATtop HANNing } [SENSe]:SGRam:FFT:WINDow?
Arguments	KAISer selects the Kaiser (RBW) window. MIL6db selects the -6 dB RBW (MIL) window. CISPr selects the CISPR window. FLATtop selects the flat-top window. HANNing selects the Hanning window. BH4B selects the Blackman-Harris 4B type window. UNIFORM selects the uniform window.
Examples	SENSe:SGRAM:FFT:WINDOW HANNing selects the Hanning window.

[SENSe]:SGRam:FILTer[:SHAPE]

Sets or queries the filter shape in the spectrogram. This command is equivalent to [\[SENSe\]:SGRam:FFT:WINDow](#).

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSe]:SGRam:FILTer[:SHAPE] { KAISer MIL6db CISPr BH4B UNIFORM FLATtop HANNing } [SENSe]:SGRam:FILTer[:SHAPE]?

Arguments KAISer selects the Kaiser (RBW) window.
 MIL6db selects the -6 dB RBW (MIL) window.
 CISPr selects the CISPR window.
 FLATtop selects the flat-top window.
 HANNing selects the Hanning window.
 BH4B selects the Blackman-Harris 4B type window.
 UNIFORM selects the uniform window.

Examples SENSE:SGRAM:FILTER:SHAPE HANNing selects the Hanning window.

[SENSe]:SGRam:FREQuency:CENTer

Sets or queries the center frequency in the spectrogram.

NOTE. *The center, start and stop frequencies are set interlocking each other with the following relationships: (start frequency) = (center frequency) - (span)/2 and (stop frequency) = (center frequency) + (span)/2.*

Conditions Measurement views: Spectrogram

Group Sense commands

Syntax [SENSe]:SGRam:FREQuency:CENTer <value>
 [SENSe]:SGRam:FREQuency:CENTer?

Related Commands [SENSe]:SGRam:FREQuency:START, [SENSe]:SGRam:FREQuency:STOP

Arguments <value>::=<Nrf> specifies the center frequency.
 Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:SGRAM:FREQUENCY:CENTER 7.5GHZ sets the center frequency to 7.5 GHz.

[SENSe]:SGRam:FREQuency:SPAN

Sets or queries the frequency span in the spectrogram.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSE]:SGRAM:FREQUENCY:SPAN <value> [SENSE]:SGRAM:FREQUENCY:SPAN?
Arguments	<value> ::= <NRF> specifies the frequency span. Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:SGRAM:FREQUENCY:SPAN 20MHZ sets the span to 20 MHz.

[SENSE]:SGRAM:FREQUENCY:SPAN:BANDwidth[:RESolution]:RATio

Sets or queries the ratio of span to RBW (Resolution Bandwidth) in the spectrogram. This command is valid when [SENSE]:SGRAM:{BANDwidth|BWIDth}[:RESolution]:AUTO is set to On.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSE]:SGRAM:FREQUENCY:SPAN:BANDwidth[:RESolution]:RATio <value> [SENSE]:SGRAM:FREQUENCY:SPAN:BANDwidth[:RESolution]:RATio?
Arguments	<value> ::= <NRF> specifies the ratio of span to RBW. Range: 20 to 1000. Programming a specified ratio sets the RBW (= span/ratio), which is rounded down to the nearest valid value.
Examples	SENSE:SGRAM:FREQUENCY:SPAN:BANDWIDTH:RESOLUTION:RATIO 200 sets the ratio to 200, setting the RBW to 200 kHz for the span of 40 MHz.

[SENSE]:SGRAM:FREQUENCY:SPAN:MAXimum (No Query Form)

Sets the frequency range to the maximum real-time span in the spectrogram.

Conditions	Measurement views: Spectrogram
-------------------	--------------------------------

Group	Sense commands
Syntax	[SENSe]:SGRam:FREQUENCY:SPAN:MAXimum <value>
Arguments	None
Examples	SENSE:SGRAM:FREQUENCY:SPAN:MAXIMUM sets the frequency range to the maximum real-time span.

[SENSe]:SGRam:FREQUENCY:START

Sets or queries the measurement start frequency (left edge of the graph) in the spectrogram.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:SGRam:FREQUENCY:CENTer](#) command.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSe]:SGRam:FREQUENCY:START <value> [SENSe]:SGRam:FREQUENCY:START?
Related Commands	[SENSe]:SGRam:FREQUENCY:STOP
Arguments	<value>::=<NRF> is the measurement start frequency. Range: (center frequency) ± (span)/2.
Examples	SENSE:SGRAM:FREQUENCY:START 6.95GHZ sets the start frequency to 6.95 GHz.

[SENSe]:SGRam:FREQUENCY:STEP

Sets or queries the frequency step size. Programming a specified step size sets [SENSe]:SGRam:FREQUENCY:STEP:AUTO OFF.

Conditions	Measurement views: Spectrogram
-------------------	--------------------------------

Group	Sense commands
Syntax	[SENSe]:SGRam:FREQUENCY:STEP <value> [SENSe]:SGRam:FREQUENCY:STEP?
Related Commands	[SENSe]:SGRam:FREQUENCY:STEP:AUTO
Arguments	<value> ::= <Nrf> specifies the frequency step size. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:SGRAM:FREQUENCY:STEP 1kHz sets the frequency step size to 1 kHz.

[SENSe]:SGRam:FREQUENCY:STEP:AUTO

Determines whether to set the frequency step size automatically or manually in the spectrogram.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSe]:SGRam:FREQUENCY:STEP:AUTO { OFF ON 0 1 } [SENSe]:SGRam:FREQUENCY:STEP:AUTO?
Arguments	OFF or 0 specifies that the frequency step size is set manually using the [SENSe]:SGRam:FREQUENCY:STEP command. ON or 1 specifies that the frequency step size is set automatically.
Examples	SENSE:SGRAM:FREQUENCY:STEP:AUTO ON specifies that the frequency step size is set automatically.

[SENSe]:SGRam:FREQUENCY:STOP

Sets or queries the measurement stop frequency (right edge of the graph) in the spectrogram.

The center, start and stop frequencies are set interlocking each other. Refer to the [SENSe]:SGRam:FREQUENCY:CENTer command.

Conditions	Measurement views: Spectrogram
Group	Sense commands
Syntax	[SENSe]:SGRam:FREQUENCY:STOP <value> [SENSe]:SGRam:FREQUENCY:STOP?
Related Commands	[SENSe]:SGRam:FREQUENCY:START
Arguments	<value> ::= <NRF> is the measurement start frequency. Range: (center frequency) ± (span)/2.
Examples	SENSE:SGRAM:FREQUENCY:STOP 7.05GHZ sets the stop frequency to 7.05 GHz.

[SENSe]:SPECTrum:{BANDwidth|BWIDth}:OPTimization

Sets or queries the method of optimizing the gain and input bandwidth in the spectrum measurement.

Conditions	Measurement views: Spectrum
Group	Sense commands
Syntax	[SENSe]:SPECTrum:{BANDwidth BWIDth}:OPTimization { AUTO MAXDynrange MINNoise MINTime } [SENSe]:SPECTrum:{BANDwidth BWIDth}:OPTimization?
Arguments	AUTO optimizes automatically the gain and input bandwidth. MAXDynrange optimizes the gain and input bandwidth to maximize the dynamic range. MINNoise optimizes the gain and input bandwidth to minimize noise. MINTime optimizes the gain and input bandwidth to minimize sweep time.
Examples	SENSE:SPECTRUM:BANDWIDTH:OPTIMIZATION AUTO optimizes automatically the gain and input bandwidth.

[SENSE]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [SENSE]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]:AUTO OFF.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSE]:SPECTrum:{BANDwidth|BWIDth}[:RESolution] <value>
[SENSE]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]?

Related Commands [SENSE]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]:AUTO

Arguments <value> ::= <NRf> specifies the RBW. Range: 1 Hz to 10 MHz.

Examples SENSE:SPECTRUM:BANDWIDTH:RESOLUTION 200kHz sets the RBW to 200 kHz.

[SENSE]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the spectrum measurement.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSE]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]:ACTual?

Arguments None

Returns <NRf> The actual RBW in Hz.

Examples SENSE:SPECTRUM:BANDWIDTH:RESOLUTION:ACTUAL? might return 299.624E+3, indicating that the actual RBW is 299.624 kHz.

[SENSe]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]:AUTO

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the spectrum measurement.

Conditions	Measurement views: Spectrum
Group	Sense commands
Syntax	[SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]:AUTO { OFF ON 0 1 } [SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]:AUTO?
Arguments	OFF or 0 specifies that the resolution bandwidth is set manually using the [SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution] command. ON or 1 specifies that the resolution bandwidth is set automatically.
Examples	SENSE:SPECTRUM:BANDWIDTH:RESOLUTION:AUTO ON sets the resolution bandwidth automatically.

[SENSe]:SPECTrum:{BANDwidth|BWIDth}[:RESolution]:MODE

Determines whether to enable or disable the RBW process.

Conditions	Measurement views: Spectrum
Group	Sense commands
Syntax	[SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]:MODE { OFF ON 0 1 } [SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]:MODE?
Arguments	OFF or 0 disables the RBW process. You can select the FFT window using the [SENSe]:SPECTrum:FFT:WINDow command. ON or 1 enables the RBW process. Refer to the [SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution] command to set the RBW.

Examples `SENSE:SPECTRUM:BANDWIDTH:RESOLUTION:MODE ON` enables the RBW process.

[SENSe]:SPECtrum:{BANDwidth|BWIDth}:VIDeo

Sets or queries the video bandwidth (VBW). Programming a specified VBW sets `[SENSe]:SPECtrum{BANDwidth|BWIDth}:VIDeo:STATe OFF`.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax `[SENSe]:SPECtrum:{BANDwidth|BWIDth}:VIDeo <value>`
`[SENSe]:SPECtrum:{BANDwidth|BWIDth}:VIDeo?`

Arguments `<value>::=<NRf>` specifies the VBW.
 Range: Current RBW/10⁴ (1 Hz minimum) to Current RBW.

Examples `SENSE:SPECTRUM:BANDWIDTH:VIDEO 200kHz` sets the VBW to 200 kHz.

[SENSe]:SPECtrum:{BANDwidth|BWIDth}:VIDeo:STATe

Determines whether to enable or disable the video bandwidth (VBW) in the spectrum measurement.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax `[SENSe]:SPECtrum:{BANDwidth|BWIDth}:VIDeo:STATe { OFF | ON`
`| 0 | 1 }`
`[SENSe]:SPECtrum:{BANDwidth|BWIDth}:VIDeo:STATe?`

Arguments OFF or 0 disables the VBW.
 ON or 1 enables the VBW.

Examples `SENSE:SPECTRUM:BANDWIDTH:VIDEO:STATE ON` enables the VBW.

[SENSE]:SPECTrum:CLEar:RESuLts (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Conditions	Measurement views: Spectrum
Group	Sense commands
Syntax	[SENSE]:SPECTrum:CLEar:RESuLts
Arguments	None
Examples	SENSE:SPECTRUM:CLEAR:RESULTS restarts multi-trace functions.

[SENSE]:SPECTrum:FFT:WINDow

Sets or queries the FFT window in the spectrum measurement. This command is equivalent to [\[SENSE\]:SPECTrum:FILTer\[:SHAPE\]](#).

Conditions	Measurement views: Spectrum
Group	Sense commands
Syntax	[SENSE]:SPECTrum:FFT:WINDow { KAISer MIL6db CISPr BH4B UNIForm FLATtop HANNing } [SENSE]:SPECTrum:FFT:WINDow?
Arguments	KAISer selects the Kaiser (RBW) window. MIL6db selects the -6 dB RBW (MIL) window. CISPr selects the CISPR window. BH4B selects the Blackman-Harris 4B type window. UNIForm selects the uniform window. FLATtop selects the flat-top window. HANNing selects the Hanning window.
Examples	SENSE:SPECTRUM:FFT:WINDOW HANNing selects the Hanning window.

[SENSe]:SPECtrum:FILTer[:SHAPE]

Sets or queries the filter shape in the spectrum measurement. This command is equivalent to [SENSe]:SPECtrum:FFT:WINDow.

Conditions	Measurement views: Spectrum
Group	Sense commands
Syntax	[SENSe]:SPECtrum:FILTer[:SHAPE] { KAISer MIL6db CISPr BH4B UNIFORM FLATtop HANNing } [SENSe]:SPECtrum:FILTer[:SHAPE]?
Arguments	KAISer selects the Kaiser (RBW) window. MIL6db selects the -6 dB RBW (MIL) window. CISPr selects the CISPR window. BH4B selects the Blackman-Harris 4B type window. UNIFORM selects the uniform window. FLATtop selects the flat-top window. HANNing selects the Hanning window.
Examples	SENSE:SPECTRUM:FILTER:SHAPE HANNing selects the Hanning window.

[SENSe]:SPECtrum:FREQuency:CENTer

Sets or queries the center frequency in the spectrum measurement.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships: $(start\ frequency) = (center\ frequency) - (span)/2$ and $(stop\ frequency) = (center\ frequency) + (span)/2$.

Conditions	Measurement views: Spectrum
Group	Sense commands
Syntax	[SENSe]:SPECtrum:FREQuency:CENTer <value> [SENSe]:SPECtrum:FREQuency:CENTer?

Related Commands [\[SENSe\]:SPECTrum:FREQuency:START](#), [\[SENSe\]:SPECTrum:FREQuency:STOP](#)

Arguments <value>::=<NRF> specifies the center frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:SPECTRUM:FREQUENCY:CENTER 7.5GHZ sets the center frequency to 7.5 GHz.

[SENSe]:SPECTrum:FREQuency:SPAN

Sets or queries the frequency span in the spectrum measurement.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSe]:SPECTrum:FREQuency:SPAN <value>
[SENSe]:SPECTrum:FREQuency:SPAN?

Arguments <value>::=<NRF> specifies the frequency span.
Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:SPECTRUM:FREQUENCY:SPAN 20MHZ sets the span to 20 MHz.

[SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio

Sets or queries the ratio of span to RBW (Resolution Bandwidth) in the spectrum measurement. This command is valid when [\[SENSe\]:SPECTrum:{BANDwidth|BWIDth}\[:RESolution\]:AUTO](#) is set to On.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio
<value>
[SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio?

Arguments `<value> ::= <NRF>` specifies the ratio of span to RBW. Range: 20 to 1000.
Programming a specified ratio sets the RBW (= span/ratio), which is rounded down to the nearest valid value.

Examples `SENSE:SPECTRUM:FREQUENCY:SPAN:BANDWIDTH:RESOLUTION:RATIO 200` sets the ratio to 200, setting the RBW to 200 kHz for the span of 40 MHz.

[SENSe]:SPECtrum:FREQuency:START

Sets or queries the measurement start frequency (left edge on the graph) in the spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:SPECtrum:FREQuency:CENTer](#) command.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax `[SENSe]:SPECtrum:FREQuency:START <value>`
`[SENSe]:SPECtrum:FREQuency:START?`

Related Commands [\[SENSe\]:SPECtrum:FREQuency:STOP](#)

Arguments `<value> ::= <NRF>` is the measurement start frequency.
Range: (center frequency) \pm (span)/2.

Examples `SENSE:SPECTRUM:FREQUENCY:START 6.95GHZ` sets the start frequency to 6.95 GHz.

[SENSe]:SPECtrum:FREQuency:STEP

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets `[SENSe]:SPECtrum:FREQuency:STEP:AUTO OFF`.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSe]:SPECTrum:FREQuency:STEP <value>
[SENSe]:SPECTrum:FREQuency:STEP?

Related Commands [\[SENSe\]:SPECTrum:FREQuency:STEP:AUTO](#)

Arguments <value>::=<NRF> specifies the frequency step size.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:SPECTRUM:FREQUENCY:STEP 1.5kHz sets the step size to 1.5 kHz.

[SENSe]:SPECTrum:FREQuency:STEP:AUTO

Determines whether to set the frequency step size automatically or manually.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSe]:SPECTrum:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[SENSe]:SPECTrum:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the [\[SENSe\]:SPECTrum:FREQuency:STEP](#) command.

ON or 1 specifies that the frequency step size is set automatically.

Examples SENSE:SPECTRUM:FREQUENCY:STEP:AUTO ON sets the frequency step size automatically.

[SENSe]:SPECTrum:FREQuency:STOP

Sets or queries the measurement stop frequency (right edge on the graph) in the spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [\[SENSe\]:SPECTrum:FREQuency:CENTer](#) command.

Conditions Measurement views: Spectrum

Group	Sense commands
Syntax	[SENSe]:SPECTrum:FREQuency:STOP <value> [SENSe]:SPECTrum:FREQuency:STOP?
Related Commands	[SENSe]:SPECTrum:FREQuency:START
Arguments	<value> := <Nrf> is the measurement start frequency. Range: (center frequency) ± (span)/2.
Examples	SENSE:SPECTRUM:FREQUENCY:STOP 7.05GHz sets the stop frequency to 7.05 GHz.

[SENSe]:SPECTrum:LENGth

Sets or queries the spectrum length when [\[SENSe\]:SPECTrum:TIME:MODE](#) is INDEPENDent. Programming a specified length sets [SENSe]:SPECTrum:LENGth:AUTO OFF.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:SPECTrum:LENGth <value> [SENSe]:SPECTrum:LENGth?
Related Commands	[SENSe]:SPECTrum:LENGth:AUTO , [SENSe]:SPECTrum:START
Arguments	<value> := <Nrf> specifies the spectrum length. Range: 0 to [(acquisition length) - (spectrum start)]. If [(spectrum start) + (spectrum length)] > (acquisition length), the actual spectrum length is reduced to the acquisition length.
Examples	SENSE:SPECTRUM:LENGTH 38.5us sets the spectrum length to 38.5 μs.

[SENSe]:SPECTrum:LENGth:ACTual? (Query Only)

Queries the actual spectrum length.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:SPECTrum:LENGth:ACTual?
Arguments	None
Returns	<NRF> Actual spectrum length in seconds.
Examples	SENSE:SPECTRUM:LENGTH:ACTUAL? might return 6.337E-6, indicating that the actual spectrum length is 6.337 μ s.

[SENSe]:SPECTrum:LENGth:AUTO

Sets or queries the spectrum length mode (automatic or manual) when [\[SENSe\]:SPECTrum:TIME:MODE](#) is INDEPENDENT.

Conditions	Measurement views: All
Group	Sense commands
Syntax	[SENSe]:SPECTrum:LENGth:AUTO { OFF ON 0 1 } [SENSe]:SPECTrum:LENGth:AUTO?
Arguments	OFF or 0 sets the spectrum length manually, using the [SENSe]:SPECTrum:LENGth command. ON or 1 sets the spectrum length automatically.
Examples	SENSE:SPECTRUM:LENGTH:AUTO ON sets the spectrum length automatically.

[SENSe]:SPECtrum:MAX:SPAN (No Query Form)

Sets the frequency span to the maximum full span instead of the maximum real-time span. For the RSA6106A Real-Time Spectrum Analyzer that is 6.2 GHz and for the / RSA6114A Real-Time Spectrum Analyzer that is 14 GHz.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSe]:SPECtrum:MAX:SPAN

Arguments None

Examples SENSE:SPECTRUM:MAX:SPAN sets the frequency span to the maximum span.

[SENSe]:SPECtrum:POINTs:COUNT

Sets or queries the number of sample points on the signal spectrum.

Conditions Measurement views: Spectrum

Group Sense commands

Syntax [SENSe]:SPECtrum:POINTs:COUNT { P801 | P2401 | P4001 | P8001
| P10401 }
[SENSe]:SPECtrum:POINTs:COUNT?

Arguments P801 sets the number of sample points to 801.
P2401 sets the number of sample points to 2401.
P4001 sets the number of sample points to 4001.
P8001 sets the number of sample points to 8001.
P10401 sets the number of sample points to 10401.

Examples SENSE:SPECTRUM:POINTS:COUNT P801 sets the number of sample points to 801.

[SENSe]:SPECTrum:START

Sets or queries the spectrum offset time when [SENSe]:SPECTrum:TIME:MODE is INDEpendent.

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:SPECTrum:START <value>
[SENSe]:SPECTrum:START?

Related Commands [SENSe]:SPECTrum:LENGth

Arguments <value> ::= <NRF> specifies the spectrum offset time.
Range: 0 to the acquisition length.
If [(spectrum start) + (spectrum length)] > (acquisition length), the actual spectrum length is reduced to the acquisition length.

Examples SENSE:SPECTRUM:START 23.5us sets the analysis offset to 23.5 μ s.

[SENSe]:SPECTrum:TIME:MODE

Sets or queries the spectrum time parameter mode (automatic or manual).

Conditions Measurement views: All

Group Sense commands

Syntax [SENSe]:SPECTrum:TIME:MODE { INDEpendent | COMMON }
[SENSe]:SPECTrum:TIME:MODE?

Related Commands [SENSe]:ANALysis commands

Arguments INDEpendent sets the spectrum time parameters manually, using the [SENSe]:SPECTrum:START and [SENSe]:SPECTrum:LENGth commands.

COMMON sets the spectrum time parameters automatically using the analysis time settings.

Examples SENSE:SPECTRUM:TIME:MODE COMMON sets the spectrum time parameters automatically.

[SENSE]:SPURious:CARRier:{BANDwidth|BWIDth}

Sets or queries the channel bandwidth for the carrier as power reference. This command is valid when [SENSE]:SPURious:REFerence is set to CARRier.

Conditions Measurement views: Spurious

Group Sense commands

Syntax [SENSE]:SPURious:CARRier:{BANDwidth|BWIDth} <value>
[SENSE]:SPURious:CARRier:{BANDwidth|BWIDth}?

Arguments <value>::=<NRF> specifies the channel bandwidth.
Range: 100 Hz to 40 MHz (Standard) / 110 MHz (Option 110).

Examples SENSE:SPURIOUS:CARRIER:BANDWIDTH 20MHZ sets the channel bandwidth to 20 MHz.

[SENSE]:SPURious:CARRier:{BANDwidth|BWIDth}:INTegration

Sets or queries the integration bandwidth to calculate the carrier power. This command is valid when [SENSE]:SPURious:REFerence is set to CARRier.

Conditions Measurement views: Spurious

Group Sense commands

Syntax [SENSE]:SPURious:CARRier:{BANDwidth|BWIDth}:INTegration
<value>
[SENSE]:SPURious:CARRier:{BANDwidth|BWIDth}:INTegration?

Arguments <value>::=<Nrf> specifies the integration bandwidth.
Range: 100 Hz to 40 MHz (Standard) / 110 MHz (Option 110).

Examples SENSE:SPURIOUS:CARRIER:BANDWIDTH:INTEGRATION 2MHZ sets the integration bandwidth to 2 MHz.

[SENSe]:SPURious:CARRier:{BANDwidth|BWIDth}[:RESolution]

Sets or queries the resolution bandwidth (RBW) to measure the carrier power. This command is valid when [SENSe]:SPURious:REFerence is set to CARRier. Programming a specified RBW sets [SENSe]:SPURious:CARRier:BANDwidth [RESolution]:AUTO OFF.

Conditions Measurement views: Spurious

Group Sense commands

Syntax [SENSe]:SPURious:CARRier:{BANDwidth|BWIDth}[:RESolution]
<value>
[SENSe]:SPURious:CARRier:{BANDwidth|BWIDth}[:RESolution]?

Related Commands [SENSe]:SPURious:CARRier:{BANDwidth|BWIDth}[:RESolution]:AUTO

Arguments <value>::=<Nrf> specifies the RBW. Range: 1 Hz to 10 MHz.

Examples SENSE:SPURIOUS:CARRIER:BANDWIDTH:RESOLUTION 200kHz sets the RBW to 200 kHz.

[SENSe]:SPURious:CARRier:{BANDwidth|BWIDth}[:RESolution]:AUTO

Determines whether to set the resolution bandwidth (RBW) automatically or manually when the power reference is set to carrier ([SENSe]:SPURious:REFerence is set to CARRier) in the Spurious measurement.

Conditions Measurement views: Spurious

Group Sense commands

Syntax	<code>[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}[:RESolution]: AUTO { OFF ON 0 1 } [SENSe]:SPURious:CARRier:{BANDwidth BWIDth}[:RESolution]: AUTO?</code>
Arguments	OFF or 0 specifies that the resolution bandwidth is set manually using the <code>[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}[:RESolution]</code> command. ON or 1 specifies that the resolution bandwidth is set automatically.
Examples	<code>SENSE:SPURIOUS:CARRIER:BANDWIDTH:RESOLUTION:AUTO ON</code> sets the resolution bandwidth automatically.

[SENSe]:SPURious:CARRier:DETEction

Sets or queries the carrier detection method. This command is valid when `[SENSe]:SPURious:REFerence` is set to CARRIER.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	<code>[SENSe]:SPURious:CARRier:DETEction { AVERage PEAK } [SENSe]:SPURious:CARRier:DETEction?</code>
Arguments	AVERage selects the average detection. PEAK selects the peak detection.
Examples	<code>SENSE:SPURIOUS:CARRIER:DETECTION PEAK</code> selects the peak detection.

[SENSe]:SPURious:CARRier:FREQuency

Sets or queries the carrier frequency in the Spurious measurement. This command is valid when `[SENSe]:SPURious:REFerence` is set to CARRIER.

Conditions	Measurement views: Spurious
Group	Sense commands

Syntax [SENSE]:SPURious:CARRier:FREQUency <value>
[SENSE]:SPURious:CARRier:FREQUency?

Arguments <value>::=<NRF> specifies the carrier frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples SENSE:SPURIOUS:CARRIER:FREQUENCY 7.5GHZ sets the carrier frequency to 7.5 GHz.

[SENSE]:SPURious:CARRier:THReshold

Sets or queries the threshold level to detect the carrier in the Spurious measurement. This command is valid when [SENSE]:SPURious:REFerence is set to CARRier.

Conditions Measurement views: Spurious

Group Sense commands

Syntax [SENSE]:SPURious:CARRier:THReshold <value>
[SENSE]:SPURious:CARRier:THReshold?

Arguments <value>::=<NRF> specifies the threshold level above which the input signal is determined to be a carrier. Range: -170 to +50 dBm. The unit can be changed by the [SENSE]:POWer:UNITs or UNIT:POWer command.

Examples SENSE:SPURIOUS:CARRIER:THRESHOLD -25 sets the carrier threshold level to -25 dBm.

[SENSE]:SPURious:CLEar:RESuLts (No Query Form)

Restarts multi-trace functions (Average and Max Hold).

Conditions Measurement views: Spurious

Group Sense commands

Syntax [SENSE]:SPURious:CLEar:RESuLts

Arguments None

Examples `SENSE:SPURIOUS:CLEAR:RESULTS` restarts multi-trace functions.

[SENSe]:SPURious[:FREQuency]:OVERlap? (Query Only)

Queries whether any of the frequency ranges (A to T) overlap, including the carrier when `[SENSe]:SPURious:REFerence` is set to `CARRier`.

NOTE. *If there are any overlaps between the ranges, the measurement will not run correctly.*

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious[:FREQuency]:OVERlap?`

Arguments None

Returns 0 (no overlap) or 1 (overlap).

Examples `SENSE:SPURIOUS:FREQUENCY:OVERLAP?` might return 1, indicating that some frequency ranges overlap.

[SENSe]:SPURious:LIST

Sets or queries how to list the spurious signals in the Spurious measurement.

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious:LIST { ALL | OVERlimit }`
`[SENSe]:SPURious:LIST?`

Arguments ALL lists all of the detected spurious signals.
OVERLimit lists the spurious signals exceeding the limits. Use the [SENSe]:SPURious:RANGe<x>:LIMit command group to set the limits.

Examples SENSE:SPURIOUS:LIST ALL lists all of the detected spurious signals.

[SENSe]:SPURious:MODE

Sets or queries the frequency range mode in the Spurious measurement.

Conditions Measurement views: Spurious

Group Sense commands

Syntax [SENSe]:SPURious:MODE { MULTi | SINGle }
 [SENSe]:SPURious:MODE?

Arguments MULTi displays all of the ranges that are enabled. Use the [SENSe]:SPURious:RANGe<x>:STATe command to enable the range.
 SINGle displays only the range that the selected spurious signal is in. Use the DISPlay:SPURious:SELEct:NUMBer command to select the spurious signal.

Examples SENSE:SPURIOUS:MODE MULTi displays all of the enabled ranges.

[SENSe]:SPURious:OPTimization

Sets or queries the method of optimizing the gain and input bandwidth in the Spurious measurement.

Conditions Measurement views: Spurious

Group Sense commands

Syntax [SENSe]:SPURious:OPTimization { AUTO | MINTime | MAXDynrange
 | MINNoise }
 [SENSe]:SPURious:OPTimization?

Arguments	AUTO optimizes automatically the gain and input bandwidth. MINTime optimizes the gain and input bandwidth to minimize sweep time. MAXDynrange optimizes the gain and input bandwidth to maximize the dynamic range. MINNoise optimizes the gain and input bandwidth to minimize noise.
Examples	SENSE:SPURIOUS:OPTIMIZATION AUTO optimizes automatically the gain and input bandwidth.

[SENSE]:SPURious:POINTs:COUNT

Sets or queries the number of sample points on the spectrum trace per range in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSE]:SPURious:POINTs:COUNT { P801 P2401 P4001 P8001 P10401 } [SENSE]:SPURious:POINTs:COUNT?
Arguments	P801 sets the trace points to 801 per range. P2401 sets the trace points to 2401 per range. P4001 sets the trace points to 4001 per range. P8001 sets the trace points to 8001 per range. P10401 sets the trace points to 10401 per range.
Examples	SENSE:SPURIOUS:POINTS:COUNT P801 sets the trace points to 801 per range.

[SENSE]:SPURious:RANGe<x>:BANDwidth:VIDeo

Sets or queries the video bandwidth (VBW) in the specified frequency range. Programming a specified VBW sets [SENSE]:SPURious:BANDwidth:VIDeo STATE OFF.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo <value> [SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo?
Related Commands	[SENSe]:SPECtrum:{BANDwidth BWIDth}:VIDeo:STATe
Arguments	<value>::=<NRF> specifies the VBW. Range: Current RBW/10 ⁴ (1 Hz minimum) to Current RBW.
Examples	SENSE:SPURIOUS:RANGE1:BANDWIDTH:VIDEO 200kHz sets the VBW to 200 kHz for Range A.

[SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo:STATe

Determines whether to enable or disable the video bandwidth (VBW) in the specified frequency range.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo:STATe { OFF ON 0 1 } [SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo:STATe?
Arguments	OFF or 0 disables the VBW. ON or 1 enables the VBW.
Examples	SENSE:SPURIOUS:RANGE1:BANDWIDTH:VIDEO:STATE ON enables the VBW for Range A.

[SENSe]:SPURious:RANGe<x>:DETection

Sets or queries the spurious detection method in the specified frequency range.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSe]:SPURious:RANGe<x>:DETection { AVERAge PEAK QUASipeak CAVERage CPEak } [SENSe]:SPURious:RANGe<x>:DETection?
Arguments	AVERAge selects the average detection. PEAK selects the peak detection. QUASipeak selects the quasi-peak detection. CAVERage selects the CISPR average detection. CPEak selects the CISPR peak detection.
Examples	SENSE:SPURIOUS:RANGE1:DETECTION PEAK selects the peak detection for Range A.

[SENSe]:SPURious:RANGe<x>:EXCURsion

Sets or queries the excursion level (how far down the signal must drop between spurious emissions) in the specified frequency range.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSe]:SPURious:RANGe<x>:EXCURsion <value> [SENSe]:SPURious:RANGe<x>:EXCURsion?
Arguments	<value> ::= <NRF> specifies the excursion level. A signal with amplitude less than the excursion level is considered to be a noise. Range: 1 to 50 dB.

Examples `SENSE:SPURIOUS:RANGE1:EXCURSION 8` sets the excursion level to 8 dB.

[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]

Sets or queries the filter shape to search the specified frequency range for spurious signals.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE] { RBW | MIL6db | CISPr }`
`[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]?`

Arguments RBW selects the RBW filter.
 MIL6db selects the -6 dB RBW (MIL) filter.
 CISPr selects the CISPR filter.

Examples `SENSE:SPURIOUS:RANGE1:FILTER:SHAPE CISPr` uses the CISPR filter in Range A.

[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]:BANDwidth

Sets or queries the filter bandwidth to search the specified frequency range for spurious signals.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]:BANDwidth <value>`
`[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]:BANDwidth?`

Arguments	<p><code><value> ::= <NRF></code> specifies the filter bandwidth.</p> <p>The setting range varies depending on the center frequency and trace detector when using the CISPR filters and detectors. Otherwise, the bandwidth minimum is a function of the span (= (stop frequency) - (start frequency)) of the range and the maximum is fixed at 5 MHz.</p> <p>By default, the value is set automatically (<code>[SENSE]:SPURIOUS:RANGE<x>:FILTER[:SHAPE]:BANDWIDTH:AUTO</code> is ON). When the detection is set to CISPR QPk (<code>[SENSE]:SPURIOUS:RANGE<x>:DETECTION</code> is QUASipeak), only one value is allowed, which is set automatically.</p>
Examples	<p><code>SENSE:SPURIOUS:RANGE1:FILTER:SHAPE:BANDWIDTH 200kHz</code> sets the filter bandwidth to 200 kHz for Range A.</p>

`[SENSE]:SPURIOUS:RANGE<x>:FILTER[:SHAPE]:BANDWIDTH:AUTO`

Determines whether to set the filter bandwidth automatically or manually for the specified frequency in the Spurious measurement.

The parameter `<x>` = 1 to 20, representing Range A to T, respectively.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	<pre>[SENSE]:SPURIOUS:RANGE<x>:FILTER[:SHAPE]:BANDWIDTH:AUTO { OFF ON 0 1 } [SENSE]:SPURIOUS:RANGE<x>:FILTER[:SHAPE]:BANDWIDTH:AUTO?</pre>
Arguments	<p>OFF or 0 specifies that the filter bandwidth is set manually using the <code>[SENSE]:SPURIOUS:RANGE<x>:FILTER[:SHAPE]:BANDWIDTH</code> command.</p> <p>ON or 1 specifies that the filter bandwidth is set automatically.</p>
Examples	<p><code>SENSE:SPURIOUS:RANGE1:FILTER:SHAPE:BANDWIDTH:AUTO ON</code> sets the filter bandwidth automatically for Range A.</p>

`[SENSE]:SPURIOUS:RANGE<x>:FREQUENCY:START`

Sets or queries the start frequency of the specified range in the Spurious measurement.

The parameter `<x>` = 1 to 20, representing Range A to T, respectively.

NOTE. The frequency ranges must not be overlapped. Use the [\[SENSe\]:SPURious\[:FREQuency\]:OVERlap?](#) query to check whether there is any overlap.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSe]:SPURious:RANGe<x>:FREQuency:START <value> [SENSe]:SPURious:RANGe<x>:FREQuency:START?
Arguments	<value>::=<Nrf> specifies the start frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	SENSE:SPURIOUS:RANGE1:FREQUENCY:START 1.615GHZ sets the start frequency of Range A to 1.615 GHz.

[SENSe]:SPURious:RANGe<x>:FREQuency:STOP

Sets or queries the stop frequency of the specified range in the Spurious measurement.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

NOTE. The frequency ranges must not be overlapped. Use the [\[SENSe\]:SPURious\[:FREQuency\]:OVERlap?](#) query to check whether there is any overlap.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSe]:SPURious:RANGe<x>:FREQuency:STOP <value> [SENSe]:SPURious:RANGe<x>:FREQuency:STOP?
Arguments	<value>::=<Nrf> specifies the stop frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Examples `SENSE:SPURIOUS:RANGE1:FREQUENCY:STOP 1.715GHZ` sets the stop frequency of Range A to 1.715 GHz.

[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:START

Sets or queries the absolute amplitude of the limits at the start (left edge) of the specified range in the Spurious measurement. This command is valid when [\[SENSe\]:SPURious:RANGe<x>:LIMit:MASK](#) is set to ABS, AND, or OR.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:START <value>`
`[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:START?`

Arguments `<value>::=<Nrf>` specifies the absolute start amplitude of the limits.
 Range: -170 to +50 dBm.
 The unit can be changed by the [\[SENSe\]:POWER:UNITs](#) or [UNIT:POWER](#) command.

Examples `SENSE:SPURIOUS:RANGE1:LIMIT:ABSOLUTE:START -30` sets the absolute start amplitude of the limits for Range A to -30 dBm.

[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:STOP

Sets or queries the absolute amplitude of the limits at the stop (right edge) of the specified range in the Spurious measurement. This command is valid when [\[SENSe\]:SPURious:RANGe<x>:LIMit:MASK](#) is set to ABS, AND, or OR.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:STOP <value>`
`[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:STOP?`

Related Commands [\[SENSe\]:POWer:UNITs](#), [UNIT:POWer](#)

Arguments <value> ::= <NRF> specifies the absolute stop amplitude of the limits.
 Range: -170 to +50 dBm.
 The unit can be changed by the [\[SENSe\]:POWer:UNITs](#) or [UNIT:POWer](#) command.

Examples `SENSE:SPURIOUS:RANGE1:LIMIT:ABSOLUTE:STOP -10` sets the absolute stop amplitude of the limits for Range A to -10 dBm.

[SENSe]:SPURious:RANGe<x>:LIMit:MASK

Sets or queries the limit mask function mode for the specified range in the Spurious measurement.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious:RANGe<x>:LIMit:MASK { ABS | REL | AND | OR | OFF }`
`[SENSe]:SPURious:RANGe<x>:LIMit:MASK?`

Arguments The following table lists the arguments.

Table 2-45: Limit mask mode

Argument	Description
ABS	Failure is detected when one of the spurious signals is larger than the absolute amplitude limit.
REL	Failure is detected when one of the spurious signals is larger than the relative amplitude limit.
AND	Failure is detected when one of the spurious signals is larger than the absolute AND relative amplitude limits.
OR	Failure is detected when one of the spurious signals is larger than the absolute OR relative amplitude limit.
OFF	Disables the mask.

To set the absolute amplitude limits, use the [\[SENSe\]:SPURious:RANGe<x>:LIMit:ABSolute:START](#) and [\[SENSe\]:SPURious:RANGe<x>:LIMit:ABSolute:STOP](#) commands.

To set the relative amplitude limits, use the [\[SENSe\]:SPURious:RANGe<x>:LIMit:RELative:START](#) and [\[SENSe\]:SPURious:RANGe<x>:LIMit:RELative:STOP](#) commands.

Examples `SENSE:SPURIOUS:RANGE1:LIMIT:MASK ABS` specifies that failure is detected when one of the spurious signals is larger than the absolute amplitude limit in Range A.

[\[SENSe\]:SPURious:RANGe<x>:LIMit:RELative:START](#)

Sets or queries the relative amplitude of the limits at the start (left edge) of the specified range in the Spurious measurement. This command is valid when [\[SENSe\]:SPURious:RANGe<x>:LIMit:MASK](#) is set to REL, AND, or OR.

The parameter `<x>` = 1 to 20, representing Range A to T, respectively.

Conditions Measurement views: Spurious

Group Sense commands

Syntax `[SENSe]:SPURious:RANGe<x>:LIMit:RELative:START <value>`
`[SENSe]:SPURious:RANGe<x>:LIMit:RELative:START?`

Arguments `<value> ::= <NRF>` specifies the relative start amplitude of the limits.
 Range: -100 to 0 dB.

Use the [\[SENSe\]:SPURious:REFerence](#) command to select the power reference.

Examples `SENSE:SPURIOUS:RANGE1:LIMIT:RELATIVE:START -30` sets the relative start amplitude of the limits for Range A to -30 dB.

[\[SENSe\]:SPURious:RANGe<x>:LIMit:RELative:STOP](#)

Sets or queries the relative amplitude of the limits at the stop (right edge) of the specified range in the Spurious measurement. This command is valid when [\[SENSe\]:SPURious:RANGe<x>:LIMit:MASK](#) is set to REL, AND, or OR.

The parameter `<x>` = 1 to 20, representing Range A to T, respectively.

Conditions Measurement views: Spurious

Group	Sense commands
Syntax	[SENSE]:SPURious:RANGe<x>:LIMit:RELAtive:STOP <value> [SENSE]:SPURious:RANGe<x>:LIMit:RELAtive:STOP?
Arguments	<value> ::= <NRF> specifies the relative stop amplitude of the limits. Range: -100 to 0 dB. Use the [SENSE]:SPURious:REFerence command to select the power reference.
Examples	SENSE:SPURIOUS:RANGE1:LIMIT:RELATIVE:STOP -10 sets the relative stop amplitude of the limits for Range A to -10 dB.

[SENSE]:SPURious:RANGe<x>:STATe

Determines whether to enable or disable the frequency range in the Spurious measurement.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSE]:SPURious:RANGe<x>:STATe { OFF ON 0 1 } [SENSE]:SPURious:RANGe<x>:STATe?
Arguments	OFF or 0 disables the frequency range. ON or 1 enables the frequency range.
Examples	SENSE:SPURIOUS:RANGE1:STATE ON enables Range A.

[SENSE]:SPURious:RANGe<x>:THReshold

Sets or queries the threshold level to detect spurious signals in the specified frequency range.

The parameter <x> = 1 to 20, representing Range A to T, respectively.

Conditions	Measurement views: Spurious
-------------------	-----------------------------

Group	Sense commands
Syntax	[SENSe]:SPURious:RANGe<x>:THReshold <value> [SENSe]:SPURious:RANGe<x>:THReshold?
Arguments	<value> ::= <NRF> specifies the threshold level above which the signal is determined to be spurious. Range: -50 to +30 dBm. The unit can be changed by the [SENSe]:POWer:UNITs or UNIT:POWer command.
Examples	SENSE:SPURIOUS:RANGE1:THRESHOLD -25 sets the threshold level to -25 dBm in Range A.

[SENSe]:SPURious:REFerence

Sets or queries the power reference in the Spurious measurement.

Conditions	Measurement views: Spurious
Group	Sense commands
Syntax	[SENSe]:SPURious:REFerence { CARRier MANUal NONE } [SENSe]:SPURious:REFerence?
Arguments	CARRier uses the carrier as the power reference. MANUal sets the power reference using the [SENSe]:SPURious:REFerence:MANUal:POWer command. NONE uses no reference.
Examples	SENSE:SPURIOUS:REFERENCE CARRier uses the carrier as the power reference.

[SENSe]:SPURious:REFerence:MANUal:POWer

Sets or queries the reference power level in the Spurious measurement. This command is valid when [SENSe]:SPURious:REFerence is set to MANUal.

Conditions	Measurement views: Spurious
-------------------	-----------------------------

Group	Sense commands
Syntax	<code>[SENSe]:SPURious:REFerence:MANua] :POWER <value></code> <code>[SENSe]:SPURious:REFerence:MANua] :POWER?</code>
Arguments	<code><value>::=<Nrf></code> specifies the reference power level. Range: -170 to +50 dBm. The unit can be changed by the [SENSe]:POWer:UNITs or UNIT:POWer command.
Examples	<code>SENSE:SPURIOUS:REFERENCE:MANUAL:POWER -25</code> sets the reference power level to -25 dBm.

[SENSe]:TOVerview:FREQuency:CENTer

Sets or queries the center frequency in the time overview.

Conditions	Measurement views: Time overview
Group	Sense commands
Syntax	<code>[SENSe]:TOVerview:FREQuency:CENTer <value></code> <code>[SENSe]:TOVerview:FREQuency:CENTer?</code>
Arguments	<code><value>::=<Nrf></code> specifies the center frequency. Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
Examples	<code>SENSE:TOVERVIEW:FREQUENCY:CENTER 7.5GHZ</code> sets the center frequency to 7.5 GHz.

[SENSe]:TOVerview:MAXTracepoints

Sets or queries the maximum trace points in the time overview.

Conditions	Measurement views: Time overview
Group	Sense commands

Syntax	<code>[SENSE]:TOVerview:MAXTracepoints { ONEK TENK HUNDredk NEVERdecimate }</code> <code>[SENSE]:TOVerview:MAXTracepoints?</code>
Arguments	ONEK sets the maximum trace points to 1 k. TENK sets the maximum trace points to 10 k. HUNDredk sets the maximum trace points to 100 k. NEVERdecimate never decimates the trace points.
Examples	<code>SENSE:TOVERVIEW:MAXTRACEPOINTS TENK</code> sets the maximum trace points to 10 k.

[SENSE]:USETtings (No Query Form)

Updates the analyzer settings. This command is useful when you need to set the analyzer including the RF attenuation before taking data acquisition. Unless this command is executed, the attenuation value is not set until acquisition is taken.

Conditions	Measurement views: All
Group	Sense commands
Syntax	<code>[SENSE]:USETtings</code>
Arguments	None
Examples	<code>SENSE:USETTINGS</code> updates settings.

*SRE

Sets or queries the value of the Service Request Enable Register (SRER). Refer to Section 3, *Status and Events*, for the register information.

Conditions	Measurement views: All
Group	IEEE common commands

Syntax *SRE <value>
*SRE?

Related Commands *CLS, *ESE, *ESR?, *STB?

Arguments <value> ::= <NR1> is a value in the range from 0 to 255. The binary bits of the SRER are set according to this value. Using an out-of-range value causes an execution error.

Examples *SRE 48 sets binary 00110000 in the SRER's bits.
*SRE? might return 32, indicating that binary value 00100000 has been set in the SRER's bits.

STATus:ACPower:EVENTs? (Query Only)

Returns the current events and status conditions for the Channel power and ACPR measurement.

Conditions Measurement views: Channel power and ACPR

Group Status commands

Syntax STATus:ACPower:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"}
Where

<ecode> ::= <NR1> is the error/event code (-32768 to 32767).
<edesc> ::= <string> is the description on the error/event.
<einfo> ::= <string> is the additional information on the error/event.

If there is no error, the response is 0, "No events to report".

Examples STATus:ACPOWER:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:{AM|FM|PM}:EVENTs? (Query Only)

Returns the current events and status conditions for the AM/FM/PM measurement.

Conditions	Measurement views: AM, FM, PM
Group	Status commands
Syntax	STATus:{AM FM PM}:EVENTs?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]}"</p> <p>Where</p> <p><ecode> ::= <NR1> is the error/event code (-32768 to 32767).</p> <p><edesc> ::= <string> is the description on the error/event.</p> <p><einfo> ::= <string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	<p>STATus:AM:EVENTs? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually in the AM measurement.</p>

STATus:AVTime:EVENTs? (Query Only)

Returns the current events and status conditions for the Amplitude versus Time measurement.

Conditions	Measurement views: Amplitude versus Time
Group	Status commands
Syntax	STATus:AVTime:EVENTs?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]}"</p>

Where
`<ecode>::=<NR1>` is the error/event code (-32768 to 32767).
`<edesc>::=<string>` is the description on the error/event.
`<einfo>::=<string>` is the additional information on the error/event.
 If there is no error, the response is 0, "No events to report".

Examples `STATUS:AVTIME:EVENTS?` might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:CCDF:EVENTS? (Query Only)

Returns the current events and status conditions for the CCDF measurement.

Conditions Measurement views: CCDF

Group Status commands

Syntax `STATUS:CCDF:EVENTS?`

Arguments None

Returns `<ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"}`

Where
`<ecode>::=<NR1>` is the error/event code (-32768 to 32767).
`<edesc>::=<string>` is the description on the error/event.
`<einfo>::=<string>` is the additional information on the error/event.
 If there is no error, the response is 0, "No events to report".

Examples `STATUS:CCDF:EVENTS?` might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:CONStE:EVENTS? (Query Only)

Returns the current events and status conditions for the constellation measurement.

Conditions	Measurement views: Constellation
Group	Status commands
Syntax	STATUS:CONStE:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"} Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:CONStE:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:DIQVtime:EVENTS? (Query Only)

Returns the current events and status conditions for the Demod I&Q versus Time measurement.

Conditions	Measurement views: Demod I&Q versus Time
Group	Status commands
Syntax	STATUS:DIQVtime:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"} Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p>

If there is no error, the response is 0, "No events to report".

Examples STATUS:DIQVTIME:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:DPSA:EVENTS? (Query Only)

Returns the current events and status conditions for the DPX spectrum measurement.

Conditions Measurement views: DPX spectrum

Group Status commands

Syntax STATUS:DPSA:EVENTS?

Arguments None

Returns <ecode>,"<edesc>[<einfo>]" {,<ecode>,"<edesc>[:<einfo>]"}
 Where

<ecode> ::= <NR1>

is the error/event code (-32768 to 32767).

<edesc> ::= <string> is the description on the error/event.

<einfo> ::= <string> is the additional information on the error/event.

If there is no error, the response is 0, "No events to report".

Examples STATUS:DPSA:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:EDiagram:EVENTS? (Query Only)

Returns the current events and status conditions for the eye diagram measurement.

Conditions Measurement views: Eye diagram

Group Status commands

Syntax	STATUS:EDIagram:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"} Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:EDIAGRAM:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:EVM:EVENTS? (Query Only)

Returns the current events and status conditions for the EVM versus Time measurement.

Conditions	Measurement views: EVM versus Time
Group	Status commands
Syntax	STATUS:EVM:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"} Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>

Examples STATUS:EVM:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:FDVTime:EVENTs? (Query Only)

Returns the current events and status conditions for the Frequency deviation versus Time measurement.

Conditions Measurement views: Frequency deviation versus Time

Group Status commands

Syntax STATus:FDVTime:EVENTs?

Arguments None

Returns <code>,"<edesc>[<einfo>]"{,<code>,"<edesc>[:<einfo>]"}
 Where

Where

<code>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0, "No events to report".

Examples STATUS:FDVTIME:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:FVTime:EVENTs? (Query Only)

Returns the current events and status conditions for the Frequency versus Time measurement.

Conditions Measurement views: Frequency versus Time

Group Status commands

Syntax	STATUS:FVTime:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}</p> <p>Where</p> <p><ecode> ::= <NR1> is the error/event code (-32768 to 32767).</p> <p><edesc> ::= <string> is the description on the error/event.</p> <p><einfo> ::= <string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:FVTIME:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:IQVTime:EVENTS? (Query Only)

Returns the current events and status conditions for the RF I&Q versus Time measurement.

Conditions	Measurement views: RF I&Q versus Time
Group	Status commands
Syntax	STATUS:IQVTime:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}</p> <p>Where</p> <p><ecode> ::= <NR1> is the error/event code (-32768 to 32767).</p> <p><edesc> ::= <string> is the description on the error/event.</p> <p><einfo> ::= <string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>

Examples STATUS:IQVTIME:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:MCPower:EVENTs? (Query Only)

Returns the current events and status conditions for the MCPR (multi-carrier ACPR) measurement.

Conditions Measurement views: MCPR

Group Status commands

Syntax STATus:MCPower:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0, "No events to report".

Examples STATUS:MCPOWER:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:MERRor:EVENTs? (Query Only)

Returns the current events and status conditions for the Magnitude error versus Time measurement.

Conditions Measurement views: Magnitude error versus Time

Group Status commands

Syntax	STATUS:MERROR:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]}"</p> <p>Where</p> <p><ecode> ::= <NR1> is the error/event code (-32768 to 32767).</p> <p><edesc> ::= <string> is the description on the error/event.</p> <p><einfo> ::= <string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:MERROR:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:OBWidth:EVENTs? (Query Only)

Returns the current events and status conditions for the Occupied Bandwidth (OBW) measurement.

Conditions	Measurement views: Occupied Bandwidth
Group	Status commands
Syntax	STATUS:OBWidth:EVENTs?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]}"</p> <p>Where</p> <p><ecode> ::= <NR1> is the error/event code (-32768 to 32767).</p> <p><edesc> ::= <string> is the description on the error/event.</p> <p><einfo> ::= <string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>

Examples STATUS:OBWIDTH:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:OPERation:CONDition? (Query Only)

Returns the contents of the Operation Condition Register (OCR).

Conditions Measurement views: All

Group Status commands

Syntax STATus:OPERation:CONDition?

Arguments None

Returns <NR1> is a decimal number showing the contents of the OCR.

Examples STATUS:OPERATION:CONDITION? might return 16, showing that the bits in the OCR have the binary value 0000000000010000, which means the analyzer is in measurement.

STATus:OPERation:ENABLE

Sets or queries the enable mask of the Operation Enable Register (OENR) which allows true conditions in the Operation Event Register to be reported in the summary bit.

Conditions Measurement views: All

Group Status commands

Syntax STATus:OPERation:ENABLE <bit_value>
STATus:OPERation:ENABLE?

Arguments <bit_value>::=<NR1> is the enable mask of the OENR. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the OENR.
Range: 0 to 32767 (The most-significant bit cannot be set true.)

Examples STATUS:OPERATION:ENABLE 1 enables the ALIGNing bit.

STATUS:OPERATION:ENABLE? might return 1, showing that the bits in the OENR have the binary value 00000000 00000001, which means that the ALIGNing bit is valid.

STATus:OPERation[:EVENT]? (Query Only)

Returns the contents of the Operation Event Register (OEVr).
Reading the OEVr clears it.

Conditions Measurement views: All

Group Status commands

Syntax STATus:OPERation[:EVENT]?

Arguments None

Returns <NR1> is a decimal number showing the contents of the OEVr.

Examples STATUS:OPERATION:EVENT? might return 1, showing that the bits in the OEVr have the binary value 00000000 00000001, which means that the ALIGNing bit is set.

STATus:OPERation:NTRansition

Sets or queries the negative transition filter value of the Operation Transition Register (OTR).

Conditions Measurement views: All

Group Status commands

Syntax `STATUS:OPERation:NTRansition <bit_value>`
 `STATUS:OPERation:NTRansition?`

Arguments <bit_value> ::= <NR1> is the negative transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the OTR.
 Range: 0 to 32767 (The most-significant bit cannot be set true.)

Examples `STATUS:OPERATION:NTRANSITION #H0011` sets the negative transition filter value to #H0011.

`STATUS:OPERATION:NTRANSITION?` might return 17.

STATUS:OPERation:PTRansition

Sets or queries the positive transition filter value of the Operation Transition Register (OTR).

Conditions Measurement views: All

Group Status commands

Syntax `STATUS:OPERation:PTRansition <bit_value>`
 `STATUS:OPERation:PTRansition?`

Arguments <bit_value> ::= <NR1> is the positive transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the OTR.
 Range: 0 to 32767 (The most-significant bit cannot be set true.)

Examples `STATUS:OPERATION:PTRANSITION 0` sets the positive transition filter value to 0.

`STATUS:OPERATION:PTRANSITION?` might return 0.

STATUS:PERRor:EVENTs? (Query Only)

Returns the current events and status conditions for the Phase error versus Time measurement.

Conditions	Measurement views: Phase error versus Time
Group	Status commands
Syntax	STATUS:PERROR:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"} Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:PERROR:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:PHVTime:EVENTS? (Query Only)

Returns the current events and status conditions for the Phase versus Time measurement.

Conditions	Measurement views: Phase versus Time
Group	Status commands
Syntax	STATUS:PHVTime:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"} Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p>

If there is no error, the response is 0, "No events to report".

Examples STATUS:PHVTIME:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:PNOise:EVENTs? (Query Only)

Returns the current events and status conditions for the phase noise measurement.

Conditions Measurement views: Spurious

Group Status commands

Syntax STATus:PNOise:EVENTs?

Arguments None

Returns <ecode>,"<edesc> [<einfo>]" {,<ecode>,"<edesc>[:<einfo>]"} }

Where

<ecode> ::= <NR1> is the error/event code (-32768 to 32767).

<edesc> ::= <string> is the description on the error/event.

<einfo> ::= <string> is the additional information on the error/event.

If there is no error, the response is 0, "No events to report".

Examples STATUS:PNOISE:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:PRESet (No Query Form)

Presets the SCPI enable registers and transition registers.

Conditions Measurement views: All

Group Status commands

Syntax	STATUS:PRESet
Arguments	None
Examples	STATUS:PRESET presets the SCPI enable registers and transition registers.

STATUS:PULSE:RESULT:EVENTS? (Query Only)

Returns the current events and status conditions for the pulse table measurement.

Conditions	Measurement views: Pulse table
Group	Status commands
Syntax	STATUS:PULSE:RESuLt:EVENTS?
Arguments	None
Returns	<code><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]"}</code> Where <code><ecode> ::= <NR1></code> is the error/event code (-32768 to 32767). <code><edesc> ::= <string></code> is the description on the error/event. <code><einfo> ::= <string></code> is the additional information on the error/event. If there is no error, the response is 0, "No events to report".
Examples	STATUS:PULSE:RESULT:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:PULSE:STATISTICS:EVENTS? (Query Only)

Returns the current events and status conditions for the pulse statistics measurement.

Conditions	Measurement views: Pulse statistics
-------------------	-------------------------------------

Group	Status commands
Syntax	STATUS:PULSE:STATISTICS:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]}"</p> <p>Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:PULSE:STATISTICS:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:PULSE:TRACE:EVENTS? (Query Only)

Returns the current events and status conditions for the pulse trace measurement.

Conditions	Measurement views: Pulse trace
Group	Status commands
Syntax	STATUS:PULSE:TRACE:EVENTS?
Arguments	None
Returns	<p><ecode>,"<edesc>[<einfo>]"{,<ecode>,"<edesc>[:<einfo>]}"</p> <p>Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>

Examples STATUS:PULSE:TRACE:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:QUESTIONABLE:CALIBRATION:CONDITION? (Query Only)

Returns the contents of the questionable calibration condition register.

Conditions Measurement views: All

Group Status commands

Syntax STATUS:QUESTIONABLE:CALIBRATION:CONDITION?

Arguments None

Returns <NR1> is a decimal number showing the contents of the questionable calibration condition register.

Examples STATUS:QUESTIONABLE:CALIBRATION:CONDITION? might return 16384, showing that the bits in the questionable calibration condition register have the binary value 01000000 00000000, which means the Alignment Needed bit is set.

STATUS:QUESTIONABLE:CALIBRATION:ENABLE

Sets or queries the enable mask of the questionable calibration enable register which allows true conditions in the questionable calibration event register to be reported in the summary bit.

Conditions Measurement views: All

Group Status commands

Syntax STATUS:QUESTIONABLE:CALIBRATION:ENABLE <bit_value>
STATUS:QUESTIONABLE:CALIBRATION:ENABLE?

Arguments <bit_value>::=<NR1> is the enable mask of the questionable calibration enable register. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable calibration enable register. Range: 0 to 32767 (The most-significant bit cannot be set true.)

Examples STATUS:QUESTIONABLE:CALIBRATION:ENABLE 16384 enables the Alignment Needed bit.

STATUS:QUESTIONABLE:CALIBRATION:ENABLE? might return 16384, showing that the bits in the questionable calibration enable register have the binary value 01000000 00000000, which means that the Calibration Summary bit is valid.

STATus:QUEStionable:CALibration[:EVENT]? (Query Only)

Returns the contents of the questionable calibration event register. Reading the register clears it.

Conditions Measurement views: All

Group Status commands

Syntax STATus:QUEStionable:CALibration[:EVENT]?

Arguments None

Returns <NR1> is a decimal number showing the contents of the questionable calibration event register.

Examples STATUS:QUESTIONABLE:CALIBRATION:EVENT? might return 16384, showing that the bits in the questionable calibration event register have the binary value 01000000 00000000, which means that the Calibration Summary bit is set.

STATus:QUEStionable:CALibration:NTRansition

Sets or queries the negative transition filter value of the questionable calibration transition register.

Conditions Measurement views: All

Group Status commands

Syntax	<code>STATUS:QUESTIONABLE:CALIBRATION:NTRANSITION <bit_value></code> <code>STATUS:QUESTIONABLE:CALIBRATION:NTRANSITION?</code>
Arguments	<code><bit_value> ::= <NR1></code> is the negative transition filter value. Range: 0 to 65535.
Returns	<code><NR1></code> is a decimal number showing the contents of the questionable calibration transition register. Range: 0 to 32767 (The most-significant bit cannot be set true.)
Examples	<code>STATUS:QUESTIONABLE:CALIBRATION:NTRANSITION #H4000</code> sets the negative transition filter value to #H4000. <code>STATUS:QUESTIONABLE:CALIBRATION:NTRANSITION?</code> might return 16384.

STATUS:QUESTIONABLE:CALIBRATION:PTRANSITION

Sets or queries the positive transition filter value of the questionable calibration transition register.

Conditions	Measurement views: All
Group	Status commands
Syntax	<code>STATUS:QUESTIONABLE:CALIBRATION:PTRANSITION <bit_value></code> <code>STATUS:QUESTIONABLE:CALIBRATION:PTRANSITION?</code>
Arguments	<code><bit_value> ::= <NR1></code> is the positive transition filter value. Range: 0 to 65535.
Returns	<code><NR1></code> is a decimal number showing the contents of the questionable calibration transition register. Range: 0 to 32767 (The most-significant bit cannot be set true.)
Examples	<code>STATUS:QUESTIONABLE:CALIBRATION:PTRANSITION 0</code> sets the positive transition filter value to 0. <code>STATUS:QUESTIONABLE:CALIBRATION:PTRANSITION?</code> might return 0.

STATUS:QUESTIONABLE:CONDITION? (Query Only)

Returns the contents of the Questionable Condition Register (QCR).

Conditions	Measurement views: All
Group	Status commands
Syntax	STATUS:QUESTIONABLE:CONDITION?
Arguments	None
Returns	<NR1> is a decimal number showing the contents of the QCR.
Examples	STATUS:QUESTIONABLE:CONDITION? might return 256, showing that the bits in the QCR have the binary value 00000001 00000000, which means the Calibration Summary bit is set.

STATUS:QUESTIONABLE:ENABLE

Sets or queries the enable mask of the Questionable Enable Register (QENR) which allows true conditions in the Questionable Event Register to be reported in the summary bit.

Conditions	Measurement views: All
Group	Status commands
Syntax	STATUS:QUESTIONABLE:ENABLE <bit_value> STATUS:QUESTIONABLE:ENABLE?
Arguments	<bit_value>::=<NR1> is the enable mask of QENR. Range: 0 to 65535.
Returns	<NR1> is a decimal number showing the contents of the QENR. Range: 0 to 32767 (The most-significant bit cannot be set true.)
Examples	STATUS:QUESTIONABLE:ENABLE 256 enables the Calibration Summary bit. STATUS:QUESTIONABLE:ENABLE? might return 256, showing that the bits in the QENR have the binary value 00000001 00000000, which means that the Calibration Summary bit is valid.

STATus:QUESTionable[:EVENT]? (Query Only)

Returns the contents of the Questionable Event Register (QEVr).
Reading the QEVr clears it.

Conditions Measurement views: All

Group Status commands

Syntax STATus:QUESTionable[:EVENT]?

Arguments None

Returns <NR1> is a decimal number showing the contents of the QEVr.

Examples STATus:QUESTionable:EVENT? might return 256, showing that the bits in the QEVr have the binary value 00000001 00000000, which means that the Calibration Summary bit is set.

STATus:QUESTionable:FREQuency:CONDition? (Query Only)

Returns the contents of the questionable frequency condition register.

Conditions Measurement views: All

Group Status commands

Syntax STATus:QUESTionable:FREQuency:CONDition?

Arguments None

Returns <NR1> is a decimal number showing the contents of the questionable frequency condition register.

Examples STATus:QUESTionable:FREQuency:CONDition? might return 512, showing that the bits in the questionable frequency condition register have the binary value 00000010 00000000, which means the Locked To External Ref bit is set.

STATus:QUESTionable:FREQuency:ENABLE

Sets or queries the enable mask of the questionable frequency enable register which allows true conditions in the questionable frequency event register to be reported in the summary bit.

Conditions	Measurement views: All
Group	Status commands
Syntax	STATus:QUESTionable:FREQuency:ENABLE <bit_value> STATus:QUESTionable:FREQuency:ENABLE?
Arguments	<bit_value> ::= <NR1> is the enable mask of the questionable frequency enable register. Range: 0 to 65535.
Returns	<NR1> is a decimal number showing the contents of the questionable frequency enable register. Range: 0 to 32767 (The most-significant bit cannot be set true.)
Examples	STATus:QUESTIONABLE:FREQUENCY:ENABLE 512 enables the Locked To External Ref bit. STATus:QUESTIONABLE:FREQUENCY:ENABLE? might return 512, showing that the bits in the questionable calibration enable register have the binary value 00000010 00000000, which means that the Locked To External Ref bit is valid.

STATus:QUESTionable:FREQuency[:EVENT]? (Query Only)

Returns the contents of the questionable frequency event register. Reading the register clears it.

Conditions	Measurement views: All
Group	Status commands
Syntax	STATus:QUESTionable:FREQuency[:EVENT]?
Arguments	None

Returns <NR1> is a decimal number showing the contents of the questionable frequency event register.

Examples STATUS:QUESTIONABLE:FREQUENCY:EVENT? might return 512, showing that the bits in the questionable frequency event register have the binary value 00000010 00000000, which means that the Locked To External Ref bit is set.

STATus:QUESTionable:FREQuency:NTRansition

Sets or queries the negative transition filter value of the questionable frequency transition register.

Conditions Measurement views: All

Group Status commands

Syntax STATus:QUESTionable:FREQuency:NTRansition <bit_value>
STATus:QUESTionable:FREQuency:NTRansition?

Arguments <bit_value> ::= <NR1> is the negative transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable frequency transition register. Range: 0 to 32767 (The most-significant bit cannot be set true.)

Examples STATUS:QUESTIONABLE:FREQUENCY:NTRANSITION #H0200 sets the negative transition filter value to #H0200.

STATUS:QUESTIONABLE:FREQUENCY:NTRANSITION? might return 512.

STATus:QUESTionable:FREQuency:PTRansition

Sets or queries the positive transition filter value of the questionable frequency transition register.

Conditions Measurement views: All

Group Status commands

Syntax `STATUS:QUESTIONABLE:FREQUENCY:PTRANSITION <bit_value>`
 `STATUS:QUESTIONABLE:FREQUENCY:PTRANSITION?`

Arguments `<bit_value>::=<NR1>` is the positive transition filter value. Range: 0 to 65535.

Returns `<NR1>` is a decimal number showing the contents of the questionable frequency transition register. Range: 0 to 32767 (The most-significant bit cannot be set true.)

Examples `STATUS:QUESTIONABLE:FREQUENCY:PTRANSITION 0` sets the positive transition filter value to 0.

 `STATUS:QUESTIONABLE:FREQUENCY:PTRANSITION?` might return 0.

STATUS:QUESTIONABLE:NTRANSITION

Sets or queries the negative transition filter value of the Questionable Transition Register (QTR).

Conditions Measurement views: All

Group Status commands

Syntax `STATUS:QUESTIONABLE:NTRANSITION <bit_value>`
 `STATUS:QUESTIONABLE:NTRANSITION?`

Arguments `<bit_value>::=<NR1>` is the negative transition filter value. Range: 0 to 65535.

Returns `<NR1>` is a decimal number showing the contents of the QTR.
Range: 0 to 32767 (The most-significant bit cannot be set true.)

Examples `STATUS:QUESTIONABLE:NTRANSITION #H0020` sets the negative transition filter value to #H0020.

 `STATUS:QUESTIONABLE:NTRANSITION?` might return 32.

STATUS:QUESTIONABLE:PTRANSITION

Sets or queries the positive transition filter value of the Questionable Transition Register (QTR).

Conditions	Measurement views: All
Group	Status commands
Syntax	<pre> STATUS:QUESTIONABLE:PTRANSITION <bit_value> STATUS:QUESTIONABLE:PTRANSITION? </pre>
Arguments	<bit_value> ::= <NR1> is the positive transition filter value. Range: 0 to 65535.
Returns	<NR1> is a decimal number showing the contents of the QTR. Range: 0 to 32767 (The most-significant bit cannot be set true.)
Examples	<pre> STATUS:QUESTIONABLE:PTRANSITION 0 </pre> sets the positive transition filter value to 0. <pre> STATUS:QUESTIONABLE:PTRANSITION? </pre> might return 0.

STATUS:SGRAM:EVENTS? (Query Only)

Returns the current events and status conditions for the spectrogram measurement.

Conditions	Measurement views: Spectrogram
Group	Status commands
Syntax	<pre> STATUS:SGRAM:EVENTS? </pre>
Arguments	None
Returns	<pre> <ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"} </pre> <p>Where</p> <ul style="list-style-type: none"> <ecode> ::= <NR1> is the error/event code (-32768 to 32767). <edesc> ::= <string> is the description on the error/event. <einfo> ::= <string> is the additional information on the error/event. <p>If there is no error, the response is 0, "No events to report".</p>

Examples STATUS:SGRAM:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:SPECTrum:EVENTs? (Query Only)

Returns the current events and status conditions and status conditions for the spectrum measurement.

Conditions Measurement views: Spectrum

Group Status commands

Syntax STATus:SPECTrum:EVENTs?

Arguments None

Returns <ecode>,"<edesc> [<einfo>]" { , <ecode>,"<edesc> [:<einfo>]"}
Where

Where

<ecode> ::= <NR1> is the error/event code (-32768 to 32767).

<edesc> ::= <string> is the description on the error/event.

<einfo> ::= <string> is the additional information on the error/event.

If there is no error, the response is 0, "No events to report".

Examples STATUS:SPECTRUM:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:SPURious:EVENTs? (Query Only)

Returns the current events and status conditions for the Spurious measurement.

Conditions Measurement views: Spurious

Group Status commands

Syntax STATus:SPURious:EVENTs?

Arguments	None
Returns	<pre><ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}</pre> <p>Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:SPURIOUS:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATUS:SQUALITY:EVENTS? (Query Only)

Returns the current events and status conditions for the signal quality measurement.

Conditions	Measurement views: Signal quality
Group	Status commands
Syntax	STATUS:SQUALITY:EVENTS?
Arguments	None
Returns	<pre><ecode>,"<edesc>[<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}</pre> <p>Where <ecode>::=<NR1> is the error/event code (-32768 to 32767). <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.</p> <p>If there is no error, the response is 0, "No events to report".</p>
Examples	STATUS:SQUALITY:EVENTS? might return 12026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

STATus:TDIagram:EVENTs? (Query Only)

Returns the current events and status conditions for the trellis diagram measurement.

Conditions Measurement views: Trellis diagram

Group Status commands

Syntax STATus:TDIagram:EVENTs?

Arguments None

Returns <ecode>, "<edesc> [<einfo>]" {, <ecode>, "<edesc>[:<einfo>]"}
Where

Where

<ecode> ::= <NR1> is the error/event code (-32768 to 32767).

<edesc> ::= <string> is the description on the error/event.

<einfo> ::= <string> is the additional information on the error/event.

If there is no error, the response is 0, "No events to report".

Examples STATus:TDIAGRAM:EVENTS? might return 12026, "Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

*STB? (Query Only)

Returns the contents of the Status Byte Register (SBR) in the status/event reporting structure using the Master Summary Status (MSS) bit. Refer to Section 3, *Status and Events*, for the register information.

Conditions Measurement views: All

Group IEEE common commands

Syntax *STB?

Related Commands [*CLS](#), [*ESE](#), [*ESR?](#), [*SRE](#)

Arguments	None
Returns	<NR1> representing the contents of the SBR as a decimal number.
Examples	*STB? might return 96, indicating that the SBR contains binary 0110 0000.

SYSTem:COMMunicate:GPIB[:SELF]:ADDRess

Sets or queries the GPIB address of the instrument.

Conditions	Measurement views: All
Group	System commands
Syntax	SYSTem:COMMunicate:GPIB[:SELF]:ADDRess <value> SYSTem:COMMunicate:GPIB[:SELF]:ADDRess?
Arguments	<value> ::= <NR1> specifies the GPIB address of the instrument. *RST has no effect on the value.
Examples	SYSTem:COMMunicate:GPIB:SELF:ADDRess 18 sets the GPIB address to 18.

SYSTem:DATE

Sets or queries the date (year, month, and day). This command is equivalent to the date setting through the Windows Control Panel.

Conditions	Measurement views: All
Group	System commands
Syntax	SYSTem:DATE <year>, <month>, <day> SYSTem:DATE?

Related Commands [SYSTem:TIME](#)

Arguments <year>::=<NRf> specifies the year (4 digits). Range: 2000 to 2099.
 <month>::=<NRf> specifies the month. Range: 1 (January) to 12 (December).
 <day>::=<NRf> specifies the day. Range: 1 to 31.
 These values are rounded to the nearest integer.
 *RST has no effect on the settings.

Examples SYSTEM:DATE 2008,3,19 sets the internal calendar to March 19, 2008.

SYSTem:ERRor:ALL? (Query Only)

Queries the error/event queue for all the unread items and removes them from the queue. The response is a comma separated list of number, string pairs in FIFO order. For details of the error messages, refer to (See Table 3-16.)

Conditions Measurement views: All

Group System commands

Syntax SYSTem:ERRor:ALL?

Arguments None

Returns <ecode>,"<edesc>[;<einfo>]"{"<ecode>,"<edesc>[;<einfo>]"}
 Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).
 <edesc>::=<string> is the description on the error/event.
 <einfo>::=<string> is the detail of the error/event.

If the queue is empty, the response is 0, "No error; Queue empty - No events to report".

Examples SYSTEM:ERROR:ALL? might return -130, "Suffix error; Unrecognized suffix, INPUTMLeve1 -10dB", , indicating that the unit of the reference level is improper.

SYSTem:ERRor:CODE:ALL? (Query Only)

Queries the error/event queue for all the unread items and removes them from the queue. The response returns a comma separated list of only the error/event code numbers in FIFO order. For details of the error messages, refer to (See Table 3-16.)

Conditions	Measurement views: All
Group	System commands
Syntax	SYSTem:ERRor:CODE:ALL?
Arguments	None
Returns	<p><ecode>{ ,<ecode>}</p> <p>Where <ecode> ::= <NR1> is the error/event code, ranging from -32768 to 32767. If the queue is empty, the response is 0.</p>
Examples	SYSTem:ERRor:CODE:ALL? might return -101, -108 of the error codes.

SYSTem:ERRor:CODE[:NEXT]? (Query Only)

Queries the error/event queue for the next item and removes it from the queue. The response returns only the error/event code number omitting the string. Except for the shortened response, the query operates identically to [SYSTem:ERRor\[:NEXT\]?](#). For details of the error messages, refer to (See Table 3-16.)

Conditions	Measurement views: All
Group	System commands
Syntax	SYSTem:ERRor:CODE[:NEXT]?
Arguments	None

Returns <ecode> ::= <NR1> is the error/event code, ranging from -32768 to 32767.

Examples SYSTEM:ERROR:CODE:NEXT? might return -101 of the error code.

SYSTEM:ERROR:COUNT? (Query Only)

Queries the error/event queue for the number of unread items. As errors and events may occur at any time, more items may be present in the queue at the time it is actually read.

Conditions Measurement views: All

Group System commands

Syntax SYSTEM:ERROR:COUNT?

Arguments None

Returns <enum> ::= <NR1> is the number of errors/events.
If the queue is empty, the response is 0.

Examples SYSTEM:ERROR:COUNT? might return 2, indicating that the error/event queue contains two of unread errors/events.

SYSTEM:ERROR[:NEXT]? (Query Only)

Queries the error/event queue for the next item and removes it from the queue. The response returns the full queue item consisting of an integer and a string. For details of the error messages, refer to (See Table 3-16.)

Conditions Measurement views: All

Group System commands

Syntax SYSTEM:ERROR[:NEXT]?

Arguments	None
Returns	<ecode>,"<edesc>[;<einfo>]" Where <ecode>::=<NR1> is the error/event code, ranging from -32768 to 32767. <edesc>::=<string> is the description on the error/event. <einfo>::=<string> is the additional information on the error/event.
Examples	SYSTEM:ERROR:NEXT? might return -130, "Suffix error; Unrecognized suffix, INPUTMLeve1 -10dB", indicating that the unit is improper.

SYSTem:OPTions? (Query Only)

Queries the options installed in the analyzer. This command is equivalent to the IEEE common command ***OPT?**.

Conditions	Measurement views: All
Group	System commands
Syntax	SYSTem:OPTions?
Arguments	None
Returns	<option>::=<string> contains the comma-separated option numbers.
Examples	SYSTEM:OPTIONS? might return "01,02,20", indicating that Option 01, 02, and 20 are currently installed in the analyzer.

SYSTem:PRESet (No Query Form)

Restores the analyzer to the defaults. This command is equivalent to the **Preset** key on the front panel.

Conditions	Measurement views: All
-------------------	------------------------

Group	System commands
Syntax	SYSTem:PRESet
Arguments	None
Examples	SYSTEM:PRESET restores the analyzer to the defaults.

SYSTem:TIME

Sets or queries the time (hours, minutes, and seconds). This command is equivalent to the time setting through the Windows Control Panel.

Conditions	Measurement views: All
Group	System commands
Syntax	SYSTem:TIME <hour>, <minute>, <second> SYSTem:TIME?
Related Commands	SYSTem:DATE
Arguments	<hour> ::= <NRF> specifies the hours. Range: 0 to 23. <minute> ::= <NRF> specifies the minutes. Range: 0 to 59. <second> ::= <NRF> specifies the seconds. Range: 0 to 59. These values are rounded to the nearest integer. *RST has no effect on the settings.
Examples	SYSTEM:TIME 10,15,30 sets the time to 1015:30.

SYSTem:VERSion? (Query Only)

Returns the SCPI version number for which the analyzer complies.

Conditions	Measurement views: All
-------------------	------------------------

Group	System commands
Syntax	SYSTEM:VERSION?
Arguments	None
Returns	<NR2> has the form YYYY.V where the Ys represent the year-version (for example, 1999) and the V represents an approved revision number for that year.
Examples	SYSTEM:VERSION? might return 1999.0 for the SCPI version.

TRACe:{AM|FM|PM}

Determines whether or not to show the trace in the AM/FM/PM view.

Conditions	Measurement views: AM, FM, PM
Group	Trace commands
Syntax	TRACe:{AM FM PM} { OFF ON 0 1 } TRACe:{AM FM PM}?
Arguments	OFF or 0 hides the trace in the AM, FM, or PM view. ON or 1 shows the trace in the AM, FM, or PM view.
Examples	TRACe:AM ON shows the trace in the AM view.

TRACe:{AM|FM|PM}:DETection

Sets or queries the display detector, the method to be used for decimating traces to fit the available horizontal space on screen. The number of horizontal pixels on screen is generally smaller than that of waveform data points. When actually displayed, the waveform data is therefore thinned out, according to the number of pixels, for being compressed.

Conditions	Measurement views: AM, FM, PM
-------------------	-------------------------------

Group	Trace commands
Syntax	TRACE:{AM FM PM}:DETEction { AVERAge POSitive NEGative } TRACE:{AM FM PM}:DETEction?
Arguments	AVERAge displays the average data value for each pixel. POSitive displays the maximum data value for each pixel. NEGative displays the minimum data value for each pixel.
Examples	TRACE:AM:DETECTION AVERAge specifies that the trace displays the average data value for each pixel.

TRACe:{AM|FM|PM}:FREeze

Determines whether or not to freeze the trace display in the AM/FM/PM view.

Conditions	Measurement views: AM, FM, PM
Group	Trace commands
Syntax	TRACE:{AM FM PM}:FREeze { OFF ON 0 1 } TRACE:{AM FM PM}:FREeze?
Arguments	OFF or 0 updates the trace display normally. ON or 1 stops updating the trace display.
Examples	TRACE:AM:FREEZE ON freezes the trace display.

TRACe:{AM|FM|PM}:FUNCtion

Sets or queries the trace function in the AM/FM/PM view.

Conditions	Measurement views: AM, FM, PM
Group	Trace commands

Syntax	TRACe:{AM FM PM}:FUNctIon { NORMa1 } TRACe:{AM FM PM}:FUNctIon?
Arguments	NORMa1 selects the normal display.
Examples	TRACe:AM:FUNCTION NORMa1 selects the normal display in the AM view.

TRACe:CONStE:MODE

Sets or queries how to display the constellation trace.

Conditions	Measurement views: Constellation
Group	Trace commands
Syntax	TRACe:CONStE:MODE { VECTors SYMBols } TRACe:CONStE:MODE?
Arguments	VECTors connects adjacent symbol points with the signal locus. SYMBols displays individual symbol points.
Examples	TRACe:CONStE:MODE VECTors shows the constellation connecting adjacent symbol points with the signal locus.

TRACe:DIQVtime:ENABle:I

Determines whether to show or hide the I trace in the Demod I&Q versus Time measurement.

Conditions	Measurement views: Demod I&Q versus Time
Group	Trace commands
Syntax	TRACe:DIQVtime:ENABle:I { OFF ON 0 1 } TRACe:DIQVtime:ENABle:I?

- Arguments** OFF or 0 hides the I trace.
ON or 1 shows the I trace.
- Examples** TRACE:DIQVTIME:ENABLE:I ON shows the I trace in the Demod I&Q versus Time measurement.

TRACe:DIQVtime:ENABLe:Q

Determines whether to show or hide the Q trace in the Demod I&Q versus Time measurement.

- Conditions** Measurement views: Demod I&Q versus Time
- Group** Trace commands
- Syntax** TRACe:DIQVtime:ENABLe:Q { OFF | ON | 0 | 1 }
TRACe:DIQVtime:ENABLe:Q?
- Arguments** OFF or 0 hides the Q trace.
ON or 1 shows the Q trace.
- Examples** TRACE:DIQVTIME:ENABLe:Q ON shows the Q trace in the Demod I&Q versus Time measurement.

TRACe:DIQVtime:SElect:I

Selects the I trace in the Demod I&Q versus Time. The query version of this command returns whether the I trace is selected or not.

- Conditions** Measurement views: Demod I&Q versus Time
- Group** Trace commands
- Syntax** TRACe:DIQVtime:SElect:I
TRACe:DIQVtime:SElect:I?
- Arguments** None

Returns { 0 | 1 }

0 indicates that the I trace is deselected.

1 indicates that the I trace is selected.

Examples TRACE:DIQVTIME:SELECT:I selects the I trace in the Demod I&Q versus Time.

TRACe:DIQVtime:SElect:Q

Selects the Q trace in the Demod I&Q versus Time. The query version of this command returns whether the Q trace is selected or not.

Conditions Measurement views: Demod I&Q versus Time

Group Trace commands

Syntax TRACe:DIQVtime:SElect:Q
TRACe:DIQVtime:SElect:Q?

Arguments None

Returns { 0 | 1 }

0 indicates that the Q trace is deselected.

1 indicates that the Q trace is selected.

Examples TRACE:DIQVTIME:SELECT:Q selects the Q trace in the Demod I&Q versus Time.

TRACe:EDIagram:ENABle:I

Determines whether to show or hide the I trace in the eye diagram.

Conditions Measurement views: Eye diagram

Group Trace commands

Syntax TRACe:EDIagram:ENABle:I { OFF | ON | 0 | 1 }
TRACe:EDIagram:ENABle:I?

Arguments OFF or 0 hides the I trace.
ON or 1 shows the I trace.

Examples TRACE:EDIAGRAM:ENABLE:I ON shows the I trace in the eye diagram.

TRACe:EDiagram:ENABLe:Q

Determines whether to show or hide the Q trace in the eye diagram.

Conditions Measurement views: Eye diagram

Group Trace commands

Syntax TRACe:EDIagram:ENABLe:Q { OFF | ON | 0 | 1 }
TRACe:EDIagram:ENABLe:Q?

Arguments OFF or 0 hides the Q trace.
ON or 1 shows the Q trace.

Examples TRACE:EDIAGRAM:ENABLE:Q ON shows the Q trace in the eye diagram.

TRACe:EDiagram:SELEct:I

Selects the I trace in the eye diagram. The query version of this command returns whether the I trace is selected or not.

Conditions Measurement views: Eye diagram

Group Trace commands

Syntax TRACe:EDIagram:SELEct:I
TRACe:EDIagram:SELEct:I?

Arguments None

Returns { 0 | 1 }

0 indicates that the I trace is deselected.

1 indicates that the I trace is selected.

Examples TRACE:EDIAGRAM:SELECT:I selects the I trace in the eye diagram.

TRACe:EDlagram:SElect:Q

Selects the Q trace in the eye diagram. The query version of this command returns whether the Q trace is selected or not.

Conditions Measurement views: Eye diagram

Group Trace commands

Syntax TRACe:EDIagram:SElect:Q
TRACe:EDIagram:SElect:Q?

Arguments None

Returns { 0 | 1 }

0 indicates that the Q trace is deselected.

1 indicates that the Q trace is selected.

Examples TRACE:EDIAGRAM:SELECT:Q selects the Q trace in the eye diagram.

TRACe:FVTime

Determines whether or not to show the trace in the Frequency versus Time view.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax TRACe:FVTime { OFF | ON | 0 | 1 }
TRACe:FVTime?

Arguments OFF or 0 hides the trace in the Frequency versus Time view.
ON or 1 shows the trace in the Frequency versus Time view.

Examples TRACE:FVTIME ON shows the trace in the Frequency versus Time view.

TRACe:FVTime:AVERAge:COUNT

Sets or queries the number of traces to combine. This command is effective when you select AVERAge with the TRACe:FVTime:FUNCTion command.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax TRACe:FVTime:AVERAge:COUNT <number>
TRACe:FVTime:AVERAge:COUNT?

Arguments <number>: :=<NR1> specifies the number of traces to combine for averaging.
Range: 1 to 10000.

Examples TRACE:FVTIME:AVERAGE:COUNT 64 sets the average count to 64.

TRACe:FVTime:COUNT

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Frequency versus Time measurement. This command is effective when TRACe:FVTime:FUNCTion is set to MAXHold or MINHold and INITiate:CONTinuous is set to OFF.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax TRACe:FVTime:COUNT <number>
TRACe:FVTime:COUNT?

Arguments <number>::=<NR1> specifies the count for Max/Min Hold.
Range: 1 to 10000.

Examples `TRACe:FVTime:COUNT 32` sets the count to 32 for the Max/Min Hold trace.

TRACe:FVTime:COUNT:ENABLE

Determines whether to enable or disable the count for the Max or Min Hold trace in the Frequency versus Time view. This command is effective when [TRACe:FVTime:FUNCTION](#) is set to MAXHold or MINHold.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax `TRACe:FVTime:COUNT:ENABle { OFF | ON | 0 | 1 }`
`TRACe:FVTime:COUNT:ENABle?`

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Examples `TRACe:FVTime:COUNT:ENABle ON` enables the Max/Min Hold count.

TRACe:FVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process in the Frequency versus Time view. This command is effective when [TRACe:FVTime:FUNCTION](#) is set to MAXHold or MINHold.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax `TRACe:FVTime:COUNT:RESet`

Arguments None

Examples `TRACe:FVTime:COUNT:RESet` clears the Max/Min Hold data and counter, and restarts the process.

TRACe:FVTime:FREeze

Determines whether or not to freeze the display of the trace in the Frequency versus Time measurement.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax `TRACe:FVTime:FREeze { OFF | ON | 0 | 1 }`
`TRACe:FVTime:FREeze?`

Arguments `OFF` or `0` updates the display of the trace normally.
`ON` or `1` stops updating the display of the trace.

Examples `TRACe:FVTime:FREeze ON` stops updating the display of the trace.

TRACe:FVTime:FUNction

Sets or queries the trace function in the Frequency versus Time measurement.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax `TRACe:FVTime:FUNction { NORMAl | AVERAge | MAXHOld | MINHOld }`
`TRACe:FVTime:FUNction?`

Arguments `NORMAl` selects the normal waveform display.
`AVERAge` selects the Average display that indicates the average frequency drift at each time point.
`MAXHOld` selects the Max Hold display that indicates the maximum frequency drift at each time point.

MINHOLD selects the Min Hold display that indicates the minimum frequency drift at each time point.

Examples TRACE:FVTIME:FUNCTION MAXHOLD displays the Max Hold trace in the Frequency versus Time measurement.

TRACe:IQVTime:AVERAge:COUNT

Sets or queries the number of traces to combine. This command works for both I and Q traces when you select AVERAge in the [TRACe:IQVTime:FUNCTION](#) command.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:AVERAge:COUNT <number>
TRACe:IQVTime:AVERAge:COUNT?

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging. Range: 1 to 10000.

Examples TRACe:IQVTime:AVERAge:COUNT 64 sets the average count to 64.

TRACe:IQVTime:COUNT

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the RF I&Q versus Time measurement. This command is effective when [TRACe:IQVTime:FUNCTION](#) is set to MAXHold or MINHold and [INITiate:CONTinuous](#) is set to OFF.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:COUNT <number>
TRACe:IQVTime:COUNT?

Arguments <number>::=<NR1> specifies the count for Max/Min Hold.
Range: 1 to 10000.

Examples TRACE:IQVTIME:COUNT 32 sets the count to 32 for the Max/Min Hold trace.

TRACe:IQVTime:COUNT:ENABLE

Determines whether to enable or disable the count for the Max or Min Hold trace in the RF I&Q versus Time view. This command is effective when [TRACe:IQVTime:FUNCTION](#) is set to MAXHold or MINHold.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:COUNT:ENABle { OFF | ON | 0 | 1 }
TRACe:IQVTime:COUNT:ENABle?

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Examples TRACE:IQVTIME:COUNT:ENABLE ON enables the Max/Min Hold count.

TRACe:IQVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process in the RF I&Q versus Time view. This command is effective when [TRACe:IQVTime:FUNCTION](#) is set to MAXHold or MINHold.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:COUNT:RESet

Arguments None

Examples TRACE:IQVTIME:COUNT:RESET clears the Max/Min Hold data and counter, and restarts the process.

TRACe:IQVTime:DETection

Sets or queries the detection method for the RF I&Q versus Time view.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:DETection { AVERAge | POSitive | NEGative | POSNegative | SAMPlE }
TRACe:IQVTime:DETection?

Arguments AVERAge displays the average data value for each pixel.
POSitive displays the maximum data value for each pixel.
NEGative displays the minimum data value for each pixel.
POSNegative displays the maximum and minimum data values for each pixel.
SAMPlE displays the first sample value received for each pixel.

Examples TRACE:IQVTIME:DETECTION AVERAGE enables display of the average value for each pixel.

TRACe:IQVTime:ENABle:I

Determines whether to show or hide the I trace in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:ENABle:I { OFF | ON | 0 | 1 }
TRACe:IQVTime:ENABle:I?

- Arguments** OFF or 0 hides the I trace.
ON or 1 shows the I trace.
- Examples** TRACE:IQVTIME:ENABLE:I ON shows the I trace in the RF I&Q versus Time measurement.

TRACe:IQVTime:ENABLE:Q

Determines whether to show or hide the Q trace in the RF I&Q versus Time measurement.

- Conditions** Measurement views: RF I&Q versus Time
- Group** Trace commands
- Syntax** TRACe:IQVTime:ENABLe:Q { OFF | ON | 0 | 1 }
TRACe:IQVTime:ENABLe:Q?
- Arguments** OFF or 0 hides the Q trace.
ON or 1 shows the Q trace.
- Examples** TRACE:IQVTIME:ENABLE:Q ON shows the Q trace in the IQ level versus Time measurement.

TRACe:IQVTime:FREeze

Determines whether to freeze the IQ traces in the RF I&Q versus Time measurement.

- Conditions** Measurement views: RF I&Q versus Time
- Group** Trace commands
- Syntax** TRACe:IQVTime:FREeze { OFF | ON | 0 | 1 }
TRACe:IQVTime:FREeze?

Arguments OFF or 0 updates IQ trace display normally.
ON or 1 stops updating IQ trace display.

Examples TRACE:IQVTIME:FREEZE ON freezes the IQ traces.

TRACe:IQVTime:FUNcTion

Sets or queries the trace function in the RF I&Q versus Time measurement.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:FUNcTion { NORMAl | AVERAge | MAXHOld |
MINHOld }
TRACe:IQVTime:FUNcTion?

Arguments NORMAl selects the normal waveform display.
AVERAge selects the Average display that indicates the average signal level at each time point.
MAXHOld selects the Max Hold display that indicates the maximum signal level at each time point.
MINHOld selects the Min Hold display that indicates the minimum signal level at each time point.

Examples TRACE:IQVTIME:FUNCTION MAXHOld displays the Max Hold trace in the IQ level versus Time measurement.

TRACe:IQVTime:SElect:I

Determines whether or not to select the I trace to obtain the maximum and minimum measurement results.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:SElect:I { OFF | ON | 0 | 1 }
 TRACe:IQVTime:SElect:I?

Related Commands [TRACe:IQVTime:SElect:Q](#)

Arguments OFF or 0 deselects the I trace.
 ON or 1 selects the I trace.
 Executing TRACe:IQVTime:SElect:I ON sets TRACe:IQVTime:SElect:Q OFF.

Examples TRACE:IQVTIME:SELECT:I ON selects the I trace in the RF I&Q versus Time measurement.

TRACe:IQVTime:SElect:Q

Determines whether or not to select the Q trace to obtain the maximum and minimum measurement results.

Conditions Measurement views: RF I&Q versus Time

Group Trace commands

Syntax TRACe:IQVTime:SElect:Q { OFF | ON | 0 | 1 }
 TRACe:IQVTime:SElect:Q?

Related Commands [TRACe:IQVTime:SElect:I](#)

Arguments OFF or 0 deselects the Q trace.
 ON or 1 selects the Q trace.
 Executing TRACe:IQVTime:SElect:Q ON sets TRACe:IQVTime:SElect:I OFF.

Examples TRACE:IQVTIME:SELECT:Q ON selects the Q trace in the RF I&Q versus Time measurement.

TRACe:OBW:MAXHold

Determines whether or not to perform a Max Hold on the spectrum data for the Occupied Bandwidth trace.

Conditions	Measurement views: Occupied Bandwidth
Group	Trace commands
Syntax	TRACe:OBW:MAXHo1d { OFF ON 0 1 } TRACe:OBW:MAXHo1d?
Arguments	OFF or 0 does not perform a Max Hold on the spectrum data. ON or 1 performs a Max Hold on the spectrum data.
Examples	TRACe:OBW:MAXHOLD ON performs a Max Hold on the spectrum data for the Occupied Bandwidth trace.

TRACe:PHVTime

Determines whether or not to show the trace in the Phase versus Time view.

Conditions	Measurement views: Phase versus Time
Group	Trace commands
Syntax	TRACe:PHVTime { OFF ON 0 1 } TRACe:PHVTime?
Arguments	OFF or 0 hides the trace in the Phase versus Time view. ON or 1 shows the trace in the Phase versus Time view.
Examples	TRACe:PHVTIME ON shows the trace in the Phase versus Time view.

TRACe:PHVTime:AVERAge:COUNT

Sets or queries the number of traces to combine. This command is effective when you select AVERAge with the [TRACe:PHVTime:FUNCTION](#) command.

Conditions	Measurement views: Phase versus Time
-------------------	--------------------------------------

Group	Trace commands
Syntax	TRACe:PHVTime:AVERAge:COUNT <number> TRACe:PHVTime:AVERAge:COUNT?
Arguments	<number>::=<NR1> specifies the number of traces to combine for averaging. Range: 1 to 10000.
Examples	TRACE:PHVTIME:AVERAGE:COUNT 64 sets the average count to 64.

TRACe:PHVTime:COUNT

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Phase versus Time measurement. This command is effective when [TRACe:PHVTime:FUNCTION](#) is set to MAXHold or MINHold and [INITiate:CONTinuous](#) is set to OFF.

Conditions	Measurement views: Phase versus Time
Group	Trace commands
Syntax	TRACe:PHVTime:COUNT <number> TRACe:PHVTime:COUNT?
Arguments	<number>::=<NR1> specifies the count for Max/Min Hold. Range: 1 to 10000.
Examples	TRACE:PHVTIME:COUNT 32 sets the count to 32 for the Max/Min Hold trace.

TRACe:PHVTime:COUNT:ENABLE

Determines whether to enable or disable the count for the Max or Min Hold trace in the Phase versus Time view. This command is effective when [TRACe:PHVTime:FUNCTION](#) is set to MAXHold or MINHold.

Conditions	Measurement views: Phase versus Time
Group	Trace commands

Syntax TRACE:PHVTime:COUNT:ENABle { OFF | ON | 0 | 1 }
TRACE:PHVTime:COUNT:ENABle?

Related Commands

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Examples TRACE:PHVTIME:COUNT:ENABLE ON enables the Max/Min Hold count.

TRACe:PHVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process in the Phase versus Time view. This command is effective when [TRACe:PHVTime:FUNCTION](#) is set to MAXHold or MINHold.

Conditions Measurement views: Phase versus Time

Group Trace commands

Syntax TRACe:PHVTime:COUNT:RESet

Arguments None

Examples TRACE:PHVTIME:COUNT:RESET clears the Max/Min Hold data and counter, and restarts the process.

TRACe:PHVTime:FREeze

Determines whether to freeze the trace display in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Trace commands

Syntax TRACE:PHVTime:FREEze { OFF | ON | 0 | 1 }
TRACE:PHVTime:FREEze?

Arguments OFF or 0 updates the trace display normally.
ON or 1 stops updating trace display.

Examples TRACE:PHVTIME:FREEZE ON stops updating trace display.

TRACE:PHVTime:FUNCTION

Sets or queries the trace function in the Phase versus Time measurement.

Conditions Measurement views: Phase versus Time

Group Trace commands

Syntax TRACE:PHVTime:FUNCTION { NORMAl | AVERAge | MAXHo1d | MINHo1d }
TRACE:PHVTime:FUNCTION?

Arguments NORMAl selects the normal waveform display.
AVERAge selects the Average display that indicates the average phase drift at each time point.
MAXHo1d selects the Max Hold display that indicates the maximum phase drift at each time point.
MINHo1d selects the Min Hold display that indicates the minimum phase drift at each time point.
POSnegative displays the maximum and minimum data values for each pixel.
SAMPle displays the first sample value received for each pixel.

Examples TRACE:PHVTIME:FUNCTION MAXHo1d displays the Max Hold trace in the Phase versus Time measurement.

TRACE:SGRam:DETECTION

Sets or queries the display detector (method to be used for decimating traces to fit the available horizontal space on screen). The number of horizontal pixels on

screen is generally smaller than that of waveform data points. When actually displayed, the waveform data is therefore thinned out, according to the number of pixels, for being compressed.

Conditions	Measurement views: Spectrogram
Group	Trace commands
Syntax	<code>TRACe:SGRam:DETEction { AVERage POSitive NEGative CAVERage CPEak QUASipeak }</code> <code>TRACe:SGRam:DETEction?</code>
Arguments	<p>AVERage displays the average data value for each pixel.</p> <p>POSitive displays the maximum data value for each pixel.</p> <p>NEGative displays the minimum data value for each pixel.</p> <p>CAVERage displays the CISPR average value for each pixel.</p> <p>CPEak displays the CISPR peak value for each pixel.</p> <p>QUASipeak displays the quasi-peak value for each pixel.</p>
Examples	<code>TRACe:SGRAM:DETECTION POSitive</code> displays the maximum data value for each pixel.

TRACe:SGRam:FREeze

Determines whether or not to freeze the spectrogram display.

Conditions	Measurement views: Spectrogram
Group	Trace commands
Syntax	<code>TRACe:SGRam:FREeze { OFF ON 0 1 }</code> <code>TRACe:SGRam:FREeze?</code>
Arguments	<p>OFF or 0 updates the display of the spectrogram normally.</p> <p>ON or 1 stops updating the display of the spectrogram.</p>

Examples TRACE:SGRAM:FREEZE ON freezes the spectrogram display.

TRACe:SGRam:FUNcTion

Sets or queries the trace function for the specified trace in the spectrogram.

Conditions Measurement views: Spectrogram

Group Trace commands

Syntax TRACe:SGRam:FUNcTion { NONE | AVERAge | MAXHOld | MINHOld }
TRACe:SGRam:FUNcTion?

Arguments NONE selects the normal spectrogram display.

AVERAge selects the Average display that indicates the average signal level at each frequency point.

MAXHOld selects the Max Hold display that indicates the maximum signal level at each frequency point.

MINHOld selects the Min Hold display that indicates the minimum signal level at each frequency point.

Examples TRACe:SGRAM:FUNCTION MAXHOld selects the Max Hold display for the spectrogram.

TRACe:SGRam:FUNcTion:TIME

Sets or queries the time length to combine traces for averaging in the spectrogram. This command is effective when [TRACe:SGRam:FUNcTion](#) is set to AVERAge, MAXHold or MINHold.

Conditions Measurement views: Spectrogram

Group Trace commands

Syntax TRACe:SGRam:FUNcTion:TIME <value>
TRACe:SGRam:FUNcTion:TIME?

Arguments `<value> ::= <NR1>` specifies the time length to combine traces for averaging. Range: 0.02 to 60 minutes.

Examples `TRACE:SGRAM:FUNCTION:TIME 1.5` sets the time length to 1.5 minutes to combine traces for averaging.

TRACe:SGRam:SElect:LINE

Sets or queries the number of line to send to the spectrum display.

Conditions Measurement views: Spectrogram

Group Trace commands

Syntax `TRACe:SGRam:SElect:LINE <number>`
`TRACe:SGRam:SElect:LINE?`

Related Commands [TRACe<x>:SPEctrum](#)

Arguments `<number> ::= <NR1>` specifies the number of line to send to the spectrum display. Range: 0 to the maximum line number of the spectrogram displayed on screen.

Examples `TRACE:SGRAM:SELECT:LINE 75` selects Line #75 in the spectrogram to send to the spectrum display.

TRACe:SPURious:COUNT

Sets or queries how many acquisitions run in the single acquisition mode for multi-trace functions (Max Hold and Average) in the Spurious measurement. This command is effective when [TRACe:SPURious:FUNCTION](#) is set to MAXHold or AVERage and [INITiate:CONTinuous](#) is set to OFF.

Conditions Measurement views: Spurious

Group Trace commands

Syntax `TRACe:SPURious:COUNT <number>`
`TRACe:SPURious:COUNT?`

Arguments `<number>::=<NR1>` specifies the count for multi-trace functions.
Range: 1 to 10000.

Examples `TRACE:SPURIOUS:COUNT 32` sets the count to 32 for multi-trace functions.

TRACe:SPURious:COUNT:ENABLE

Determines whether to enable or disable the count for multi-trace functions (Max Hold and Average) in the Spurious view. This command is effective when [TRACe:SPURious:FUNCTion](#) is set to MAXHold or AVERAge.

Conditions Measurement views: Spurious

Group Trace commands

Syntax `TRACe:SPURious:COUNT:ENABle { OFF | ON | 0 | 1 }`
`TRACe:SPURious:COUNT:ENABle?`

Arguments OFF or 0 disables the count for multi-trace functions.
ON or 1 enables the count for multi-trace functions.

Examples `TRACe:SPURIOUS:COUNT:ENABLE ON` enables the count for multi-trace functions.

TRACe:SPURious:COUNT:RESet (No Query Form)

Clears the multi-function (Max Hold or Average) data and counter, and restarts the process in the Spurious view. This command is effective when [TRACe:SPURious:FUNCTion](#) is set to MAXHold or AVERAge.

Conditions Measurement views: Spurious

Group Trace commands

Syntax `TRACe:SPURious:COUNT:RESet`

Arguments None

Examples TRACE:SPURIOUS:COUNT:RESET clears the multi-function data and counter, and restarts the process.

TRACe:SPURious:FREeze

Determines whether or not to freeze the display of the trace in the Spurious view.

Conditions Measurement views: Spurious

Group Trace commands

Syntax TRACe:SPURious:FREeze { OFF | ON | 0 | 1 }
TRACe:SPURious:FREeze?

Arguments OFF or 0 updates the display of the trace normally.
ON or 1 stops updating the display of the trace.

Examples TRACE:SPURIOUS:FREEZE ON stops updating the display of the trace.

TRACe:SPURious:FUNcTion

Sets or queries the trace function in the Spurious view.

Conditions Measurement views: Spurious

Group Trace commands

Syntax TRACe:SPURious:FUNcTion { NONE | MAXHOLD | AVERAGE }
TRACe:SPURious:FUNcTion?

Arguments NONE selects normal display.
MAXHOLD selects the Max Hold display that indicates the maximum amplitude drift at each frequency point.
AVERAGE selects the Average display that indicates the average amplitude drift at each frequency point.

Examples TRACE:SPURIOUS:FUNCTION MAXHold displays the Max Hold trace in the Spurious measurement.

TRACe1:TOVerview

Enables display of or queries the display status of the specified trace. Only Trace1 is valid.

Conditions Measurement views: General Waveform display

Group Trace commands

Syntax TRACe1:TOVerview { OFF | ON | 0 | 1 }
TRACe1:TOVerview?

Arguments OFF or 0 disables the trace overview.
ON or 1 enables the trace overview.

Examples TRACe1:TOVerview ON enables display of Trace1.

TRACe1:TOVerview:AVERAge:COUNT

Sets or queries the number of traces averaged to generate the specified trace. Only Trace1 is valid.

Conditions Measurement views: Trace Function set to Average

Group Trace commands

Syntax TRACe1:TOVerview:AVERAge:COUNT <value>
TRACe1:TOVerview:AVERAge:COUNT?

Arguments <value> ::= <NR1> an integer number of traces to average to create the waveform display.

Examples TRACe1:TOVerview:AVERAge:COUNT 200 sets the Average count for Trace 1 to 200.

TRACe1:TOVerview:COUNT

Enables or queries the count set for the specified trace. Only Trace1 is valid.

Conditions Measurement views: Trace Function set to Average

Group Trace commands

Syntax TRACe1:TOVerview:COUNT <value>
TRACe1:TOVerview:COUNT?

Arguments <value> ::= <NRF>

Examples TRACe1:TOVerview:COUNT 200 sets the Trace1 Average count to 200.

TRACe1:TOVerview:COUNT:ENABLE

Enables or queries the Average count for the specified trace. Only Trace1 is valid.

Conditions Measurement views: Trace Function set to Average

Group Trace commands

Syntax TRACe1:TOVerview:COUNT:ENABLE { OFF | ON | 0 | 1 }
TRACe1:TOVerview:COUNT:ENABLE?

Arguments OFF or 0 disables the trace count.
ON or 1 enables the trace count.

Examples TRACe1:TOVerview:COUNT:ENABLE ON enables the Trace1 Average count.

TRACe1:TOVerview:COUNT:RESet (No Query Form)

Resets the waveform count for the specified trace. Only Trace1 is valid..

Conditions Measurement views: Trace Function set to Average

Group	Trace commands
Syntax	TRACe1:TOVerview:COUNT:RESet
Arguments	None
Examples	TRACe1:TOVerview:COUNT:RESet sets the trace count to 1.

TRACe1:TOVerview:DETection

Enables or queries the type of detection for the specified trace. Only Trace1 is valid.

Conditions	Measurement views: all
Group	Trace commands
Syntax	TRACe1:TOVerview:DETection { AVERAge POSitive NEGative POSNegative SAMPle } TRACe1:TOVerview:DETection?
Arguments	AVERAge displays the average data value for each pixel. POSitive displays the maximum data value for each pixel. NEGative displays the minimum data value for each pixel. POSNegative displays the maximum and minimum data values for each pixel. SAMPle displays the first sample value received for each pixel.
Examples	TRACe1:TOVerview:DETection POSitive enables positive detection on Trace1.

TRACe1:TOVerview:FREeze

Enables or queries a halt to acquisition updates for the specified trace. Only Trace1 is valid.

Conditions	Measurement views: all
-------------------	------------------------

Group	Trace commands
Syntax	TRACe1:TOVerview:FREeze { OFF ON 0 1 } TRACe1:TOVerview:FREeze?
Arguments	OFF or 0 disables the trace freeze function. ON or 1 enables the trace freeze function.
Examples	TRACe1:TOVerview:FREeze ON Halts acquisition updates to Trace1.

TRACe1:TOVerview:FUNCTION

Enables or queries the selected Function for the specified trace. Only Trace1 is valid.

Conditions	Measurement views: all
Group	Trace commands
Syntax	TRACe1:TOVerview:FUNCTION { NORMAl AVERAge MAXHOld MINHOld } TRACe1:TOVerview:FUNCTION?
Arguments	NORMAl Each new trace is displayed and then replaced by the next trace.. AVERAge Multiple traces are averaged together to generate the displayed trace.. MAXHOld Displays the maximum value in the trace record for each display point. MINHOld Displays the minimum value in the trace record for each display point.
Examples	TRACe1:TOVerview:FUNCTION AVERAge enables the averaging of multiple traces on Trace1.

TRACe<x>:AVTime

Determines whether or not to show the specified trace in the Amplitude versus Time view.

The parameter <x> = 1 to 4; All traces are valid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime { OFF ON 0 1 } TRACe<x>:AVTime?
Arguments	OFF or 0 hides the specified trace in the Amplitude versus Time view. ON or 1 shows the specified trace in the Amplitude versus Time view.
Examples	TRACE1:AVTIME ON shows Trace 1 in the Amplitude versus Time view.

TRACe<x>:AVTime:AVERAge:COUNT

Sets or queries the number of traces to combine. This command is effective when you select AVERAge with the [TRACe<x>:AVTime:FUNCTion](#) command.

The parameter <x> = 1 to 3; Trace 4 (math trace) is invalid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:AVERAge:COUNT <number> TRACe<x>:AVTime:AVERAge:COUNT?
Arguments	<number> ::= <NR1> specifies the number of traces to combine for averaging. Range: 1 to 10000.
Examples	TRACE1:AVTIME:AVERAGE:COUNT 64 sets the average count to 64 for Trace 1.

TRACe<x>:AVTime:AVERAge:RESet (No Query Form)

Restarts acquisition and display of waveforms for the specified trace. For an Average, Max Hold, or Min Hold trace, it restarts the sequence, discarding accumulated data and resetting the counter.

The parameter <x> = 1 to 3; Trace 4 (math trace) is invalid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:AVERAge:RESet
Related Commands	TRACe<x>:AVTime:FUNctIon
Arguments	None
Examples	TRACE1:AVTIME:AVERAGE:RESET restarts acquisition and display of waveforms for Trace 1.

TRACe<x>:AVTime:COUNT

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Amplitude versus Time measurement. This command is effective when [TRACe<x>:AVTime:FUNctIon](#) is set to MAXHold or MINHold and [INITiate:CONTInuous](#) is set to OFF.

The parameter <x> = 1 to 3; Trace 4 (math trace) is invalid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:COUNT <number> TRACe<x>:AVTime:COUNT?
Arguments	<number>::=<NR1> specifies the count for Max/Min Hold. Range: 1 to 10000.
Examples	TRACE1:AVTIME:COUNT 32 sets the count to 32 for Trace 1.

TRACe<x>:AVTime:COUNT:ENABLE

Determines whether to enable or disable the count for the Max or Min Hold trace in the Amplitude versus Time view. This command is effective when [TRACe<x>:AVTime:FUNCTION](#) is set to MAXHold or MINHold.

The parameter <x> = 1 to 3; Trace 4 (math trace) is invalid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:COUNT:ENABle { OFF ON 0 1 } TRACe<x>:AVTime:COUNT:ENABle?
Arguments	OFF or 0 disables the count for the Max/Min Hold trace. ON or 1 enables the count for the Max/Min Hold trace.
Examples	TRACE1:AVTIME:COUNT:ENABLE ON enables the Max/Min Hold count for Trace 1.

TRACe<x>:AVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process for the specified trace in the Amplitude versus Time view. This command is effective when [TRACe<x>:AVTime:FUNCTION](#) is set to MAXHold or MINHold.

The parameter <x> = 1 to 3; Trace 4 (math trace) is invalid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:COUNT:RESet
Arguments	None
Examples	TRACE1:AVTIME:COUNT:RESET clears the Max/Min Hold data and counter, and restarts the process for Trace 1.

TRACe<x>:AVTime:DETection

Sets or queries the display detector (method to be used for decimating traces to fit the available horizontal space on screen). The number of horizontal pixels on screen is generally smaller than that of waveform data points. When actually displayed, the waveform data is therefore thinned out, according to the number of pixels, for being compressed.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:DETection { AVERAge POSitive NEGative POSNegative SAMPlE } TRACe<x>:AVTime:DETection?
Arguments	AVERAge displays the average data value for each pixel. POSitive displays the maximum data value for each pixel. NEGative displays the minimum data value for each pixel. POSNegative displays the maximum and minimum data values for each pixel. SAMPlE displays the first sample value received for each pixel.
Examples	TRACE:AVTIME:DETECTION AVERAge specifies that the trace displays the average data value for each pixel.

TRACe<x>:AVTime:FREeze

Determines whether or not to freeze the display of the specified trace in the Amplitude versus Time view.

The parameter <x> = 1 to 4; All traces are valid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:FREeze { OFF ON 0 1 } TRACe<x>:AVTime:FREeze?

Arguments OFF or 0 updates the display of the specified trace normally.
ON or 1 stops updating the display of the specified trace.

Examples TRACE1:AVTIME:FREEZE ON freezes the display for Trace 1.

TRACe<x>:AVTime:FUNCTION

Sets or queries the function for the specified trace in the Amplitude versus Time view.

The parameter <x> = 1 to 3; Trace 4 (math trace) is invalid.

Conditions Measurement views: Amplitude versus Time

Group Trace commands

Syntax TRACe<x>:AVTime:FUNCTION { NORMAl | AVERAge | MAXHOld | MINHOld }
TRACe<x>:AVTime:FUNCTION?

Arguments NORMAl selects the normal display.
AVERAge selects the Average display that indicates the average amplitude at each time point.
MAXHOld selects the Max Hold display that indicates the maximum amplitude at each time point.
MINHOld selects the Min Hold display that indicates the minimum amplitude at each time point.

Examples TRACE1:AVTIME:FUNCTION MAXHOld selects Max Hold for Trace 1 in the Amplitude versus Time view.

TRACe<x>:AVTime:LEFToperand

Sets or queries the left operand for the math trace (Trace 4) in the Amplitude versus Time view.

The parameter <x> = 4; Only Trace 4 (math trace) is valid.

Conditions Measurement views: Amplitude versus Time

Group	Trace commands
Syntax	TRACe<x>:AVTime:LEFToperand { TRACE1 TRACE2 TRACE3 } TRACe<x>:AVTime:LEFToperand?
Related Commands	TRACe<x>:AVTime:RIGHToperand
Arguments	TRACE1 selects Trace 1 as the left operand for the math trace. TRACE2 selects Trace 2 as the left operand for the math trace. TRACE3 selects Trace 3 as the left operand for the math trace.
Examples	TRACE4:AVTIME:LEFTOPERAND TRACE2 selects Trace 2 as the left operand for the math trace.

TRACe<x>:AVTime:RIGHToperand

Sets or queries the right operand for the math trace (Trace 4) in the Amplitude versus Time view.

The parameter <x> = 4; Only Trace 4 (math trace) is valid.

Conditions	Measurement views: Amplitude versus Time
Group	Trace commands
Syntax	TRACe<x>:AVTime:RIGHToperand { TRACE1 TRACE2 TRACE3 } TRACe<x>:AVTime:RIGHToperand?
Related Commands	TRACe<x>:AVTime:LEFToperand
Arguments	TRACE1 selects Trace 1 as the right operand for the math trace. TRACE2 selects Trace 2 as the right operand for the math trace. TRACE3 selects Trace 3 as the right operand for the math trace.
Examples	TRACE4:AVTIME:RIGHTOPERAND TRACE1 selects Trace 1 as the right operand for the math trace.

TRACe<x>:AVTime:SElect

Sets or queries the trace whose measurement results are being displayed in the readout on the top and bottom of the view.

The parameter <x> = 1 to 4; All traces are valid.

Conditions Measurement views: Amplitude versus Time

Group Trace commands

Syntax TRACe<x>:AVTime:SElect
TRACe<x>:AVTime:SElect?

Arguments None

Returns { 0 | 1 }

0 indicates that the results are not being displayed in the readout for the trace.

1 indicates that the results are being displayed in the readout for the trace.

Examples TRACE1:AVTIME:SELECT selects Trace 1 to display the measurement results in the readout.

TRACE1:AVTIME:SELECT? might return 1, indicating that the results are being displayed in the readout for Trace 1.

TRACe<x>:CCDF:FREeze

Determines whether or not to freeze the display of the specified trace (Trace 1 or 2) in the CCDF view.

The parameter <x> = 1 or 2; Trace 3 (Gaussian curve) is invalid.

Conditions Measurement views: CCDF

Group Trace commands

Syntax TRACe<x>:CCDF:FREeze { OFF | ON | 0 | 1 }
TRACe<x>:CCDF:FREeze?

Arguments OFF or 0 updates the display of the specified trace normally.
ON or 1 stops updating the display of the specified trace.

Examples TRACE1:CCDF:FREEZE ON freezes the display for Trace 1.

TRACe<x>:CCDF:SElect

Sets or queries the trace whose measurement results are being displayed in the readout on the top of the view. The selected trace is indicated by the measurement pointer (pink triangle) on the waveform.

The parameter <x> = 1 to 3; All traces are valid.

Conditions Measurement views: CCDF

Group Trace commands

Syntax TRACe<x>:CCDF:SElect
TRACe<x>:CCDF:SElect?

Arguments None

Returns { 0 | 1 }

0 indicates that the results are not being displayed in the readout for the trace.

1 indicates that the results are being displayed in the readout for the trace.

Examples TRACE1:CCDF:SELECT selects Trace 1 to display the measurement results in the readout.

TRACE1:CCDF:SELECT? might return 1, indicating that the results are being displayed in the readout for Trace 1.

TRACe<x>:CCDF:SHOW

Determines whether to show or hide the specified trace in the CCDF view.

The parameter <x> = 1 to 3; All traces are valid.

Conditions Measurement views: CCDF

Group	Trace commands
Syntax	TRACe<x>:CCDF:SHOW { OFF ON 0 1 } TRACe<x>:CCDF:SHOW?
Arguments	OFF or 0 hides the specified trace. ON or 1 shows the specified trace.
Examples	TRACE1:CCDF:SHOW ON shows Trace 1 in the CCDF view.

TRACe<x>:CCDF:X

Sets or queries the horizontal position of the measurement pointer (pink triangle) to measure the CCDF. Use the [TRACe<x>:CCDF:Y?](#) query to read the value.

The parameter <x> = 1 to 3.

NOTE. Use the [TRACe<x>:CCDF:SHOW](#) command to show the specified trace and the [TRACe<x>:CCDF:SElect](#) command to select the trace before running the [TRACe<x>:CCDF:X](#) command.

Conditions	Measurement views: CCDF
Group	Trace commands
Syntax	TRACe<x>:CCDF:X <value> TRACe<x>:CCDF:X?
Arguments	<value> ::= <NRf> specifies the horizontal position of the measurement pointer. Range: 0 to 20 dB.
Examples	TRACE1:CCDF:X 5 puts the measurement pointer at 5 dB on Trace 1.

TRACe<x>:CCDF:Y? (Query Only)

Queries the vertical position (CCDF value) of the measurement pointer (displayed as a pink triangle). Use the [TRACe<x>:CCDF:X](#) command to set the horizontal position of the pointer.

The parameter $\langle x \rangle = 1$ to 3.

NOTE. Use the `TRACe $\langle x \rangle$:CCDF:SHOW` command to show the specified trace and the `TRACe $\langle x \rangle$:CCDF:SElect` command to select the trace before running the `TRACe $\langle x \rangle$:CCDF:Y?` query.

Conditions	Measurement views: CCDF
Group	Trace commands
Syntax	TRACe $\langle x \rangle$:CCDF:Y?
Arguments	None
Returns	<p><code><value>::=<Nrf></code> is the vertical position (CCDF) of the measurement pointer. Range: 0 to 100%.</p> <p>The value of 99.0999953003E+36 is returned if the trace is not available.</p>
Examples	TRACE1:CCDF:Y? might return 14.72, indicating the CCDF is 14.72% at the measurement pointer on Trace 1.

TRACe $\langle x \rangle$:DPSA

Determines whether or not to show the specified trace in the DPX spectrum view. The parameter $\langle x \rangle = 1$ to 5; All traces are valid.

Conditions	Measurement views: DPX spectrum
Group	Trace commands
Syntax	<pre>TRACe$\langle x \rangle$:DPSA { OFF ON 0 1 } TRACe$\langle x \rangle$:DPSA?</pre>
Arguments	<p>OFF or 0 hides the specified trace in the DPX spectrum view.</p> <p>ON or 1 shows the specified trace in the DPX spectrum view.</p>

Examples TRACE1:DPSA ON shows Trace 1 (the maximum trace) in the DPX spectrum view.

TRACe<x>:DPSA:AVERAge:COUNT

Sets or queries the number of traces to combine for averaging in the DPX spectrum view.

The parameter <x> = 3; Only Trace 3 (average trace) is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:AVERAge:COUNT <number>
TRACe<x>:DPSA:AVERAge:COUNT?

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging. Range: 1 to 10000.

Examples TRACE3:DPSA:AVERAGE:COUNT 32 sets the average count to 32.

TRACe<x>:DPSA:COLor:CURVe

Sets or queries how colors are mapped to the signal density in the DPX spectrum bitmap display. The mapping can be linear (Curve = 1), or it can be set to concentrate the resolution on the lower level of the range (Curve > 1) or the mapping can be set to show the best resolution on the upper range of density or hit count (Curve = 0.1 – 0.99). This command is only valid for the Bitmap display.

The parameter <x> = 5; only Trace5 is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:COLor:CURVe <value>
TRACe<x>:DPSA:COLor:CURVe?

Arguments <value>::=<NRf> specifies how colors are mapped to the signal density. Range:

Examples TRACe<x>:DPSA:COLor:CURVe 1.5 concentrates the resolution on the lower level of the range on the Bitmap display.

TRACe<x>:DPSA:COLor:INTensity

Sets or queries the color intensity in the DPX spectrum view.
The value is common to all traces.

The parameter <x> = 1 to 5; All traces are valid.

Conditions Measurement views: DPX spectrum
Not valid for Option 200 instruments.

Group Trace commands

Syntax TRACe<x>:DPSA:COLor:INTensity <value>
TRACe<x>:DPSA:COLor:INTensity?

Arguments <value>::=<Nrf> specifies color intensity. Range: 1 to 100%.

Examples TRACE1:DPSA:COLOR:INTENSITY 30 sets the color intensity to 30%.

TRACe<x>:DPSA:COLor:SCALE:AUTO (No Query Form)

Automatically adjusts the Max and Min color settings to display the broadest range of colors in the DPX spectrum bitmap display. This command is only valid for the Bitmap display.

The parameter <x> = 5; only Trace5 is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:COLor:SCALE:AUTO

Arguments <x>::=5 specifies the auto-color setting for the Bitmap trace.

Examples TRACe5:DPSA:COLor:SCALE:AUTO autosets the Bitmap display color scheme.

TRACe<x>:DPSA:DETection

Sets or queries the detection type (POSitive, NEGative, AVERage) for traces 1, 2 and 3 in the DPX spectrum view.

Trace 4 (math trace) and Trace 5 (bitmap trace) are invalid choices.

Conditions Measurement views: DPX spectrum

Option 200 only

Group Trace commands

Syntax TRACe<x>:DPSA:DETection { AVERage | NEGative | POSitive }
TRACe<x>:DPSA:DETection?

Arguments The following table shows the trace function and display. For the average trace, use the [TRACe<x>:DPSA:AVERage:COUNT](#) command to set the average count.

Examples TRACE1:DPSA:DETection AVERage enables analysis to look for AVERage on Trace 1.

TRACe<x>:DPSA:DOT:PERsistent

Determines whether to enable or disable the dot persistence for the bitmap trace (Trace 5) in the DPX spectrum view.

The parameter <x> = 5; Only Trace 5 (bitmap trace) is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:DOT:PERsistent { OFF | ON | 0 | 1 }
TRACe<x>:DPSA:DOT:PERsistent?

Arguments OFF or 0 disables the dot persistence.

ON or 1 enables the dot persistence.

Examples TRACE5:DPSA:DOT:PERSISTENT ON enables the dot persistence in the DPX spectrum view.

TRACe<x>:DPSA:DOT:PERsistent:TYPE

Sets or queries the persistence type for the bitmap trace (Trace 5) in the DPX spectrum view.

The parameter <x> = 5; Only Trace 5 (bitmap trace) is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:DOT:PERsistent:TYPE { VARIable | INFInite }
TRACe<x>:DPSA:DOT:PERsistent:TYPE?

Arguments VARIable selects the variable persistence display which leaves acquired data points on the display for a period of time specified by the TRACe<x>:DPSA:DOT:PERsistent:VARIable command.

INFInite selects the infinite persistence display which accumulates data points on the display indefinitely.

Examples TRACE5:DPSA:DOT:PERSISTENT:TYPE VARIable selects the variable persistence display.

TRACe<x>:DPSA:DOT:PERsistent:VARIable

Sets or queries how long data points are displayed. This command is effective when TRACe<x>:DPSA:DOT:PERsistent:TYPE is set to VARIable. This affects the display only.

The parameter <x> = 5; Only Trace 5 (bitmap trace) is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:DOT:PERsistent:VARIable <number>
TRACe<x>:DPSA:DOT:PERsistent:VARIable?

Arguments <number>::=<NR1> specifies the how long waveform points are displayed on the screen. For instruments without Option 200 – Range: 1 to 1000 (unitless; the default value is 10). For instruments with Option 200 – Range: 100 ms to 60 s (the default value is 1.0 s). For

Examples TRACE5:DPSA:DOT:PERSISTENT:VARIABLE 20 specifies that the waveform points are displayed on the screen for a period of 20 before they disappear.

TRACe<x>:DPSA:FREEze

Determines whether or not to freeze the display of the specified trace in the DPX spectrum view.

The parameter <x> = 1 to 5; All traces are valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:FREEze { OFF | ON | 0 | 1 }
TRACe<x>:DPSA:FREEze?

Arguments OFF or 0 updates the display of the specified trace normally.
ON or 1 stops updating the display of the specified trace.

Examples TRACE1:DPSA:FREEZE ON freezes the display for the +peak trace.

TRACe<x>:DPSA:FUNction

Sets or queries the trace function for the +Peak, -Peak, or Average trace (Trace 1, 2, or 3, respectively) in the DPX spectrum view.

The parameter <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (bitmap trace) are invalid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:FUNCTION { NORMAl | HOLD | AVERAge }
TRACe<x>:DPSA:FUNCTION?

Arguments The following table shows the trace function and display. For the average trace, use the [TRACe<x>:DPSA:AVERAge:COUNT](#) command to set the average count.

Function	Trace1 (+Peak trace)	Trace2 (-Peak trace)	Trace3 (Average trace)
NORMAl	Normal spectrum (Detection: +Peak)	Normal spectrum (Detection: -Peak)	Normal spectrum (Detection: Average)
HOLD	Max-hold spectrum	Min-hold spectrum	NA
AVERAge	NA	NA	Average spectrum

Examples TRACE1:DPSA:FUNCTION HOLD selects the max hold waveform for Trace 1.

TRACe<x>:DPSA:LEFToperand

Sets or queries the left operand for the math trace (Trace 4) in the DPX spectrum view. With Option 200, trace detection is not configurable.

The parameter <x> = 4; Only Trace 4 (math trace) is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:LEFToperand { TRACe1 | TRACe2 | TRACe3 }
TRACe<x>:DPSA:LEFToperand?

Related Commands [TRACe<x>:DPSA:RIGHToperand](#)

Arguments TRACE1 selects Trace 1 as the left operand for the math trace.
TRACE2 selects Trace 2 as the left operand for the math trace.
TRACE3 selects Trace 3 as the left operand for the math trace.

Examples TRACE4:DPSA:LEFTOPERAND TRACE2 selects Trace 2 as the left operand for the math trace.

TRACe<x>:DPSA:RIGHtooperand

Sets or queries the right operand for the math trace (Trace 4) in the DPX spectrum view. With Option 200, trace detection is not configurable.

The parameter <x> = 4; Only Trace 4 (math trace) is valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:RIGHtooperand { TRACE1 | TRACE2 | TRACE3 }
TRACe<x>:DPSA:RIGHtooperand?

Related Commands [TRACe<x>:DPSA:LEFTooperand](#)

Arguments TRACE1 selects Trace 1 as the right operand for the math trace.

TRACE2 selects Trace 2 as the right operand for the math trace.

TRACE3 selects Trace 3 as the right operand for the math trace.

Examples TRACE4:DPSA:RIGHTOPERAND TRACE1 selects Trace 1 as the right operand for the math trace.

TRACe<x>:DPSA:SElect

Sets or queries the trace to display the readout at the upper left of the DPX spectrum view.

The parameter <x> = 1 to 5; All traces are valid.

Conditions Measurement views: DPX spectrum

Group Trace commands

Syntax TRACe<x>:DPSA:SElect
TRACe<x>:DPSA:SElect?

Arguments None

Returns { 0 | 1 }

0 indicates that the readout is not being displayed for the specified trace.
1 indicates that the readout is being displayed for the specified trace.

Examples TRACE1:DPSA:SELECT selects Trace 1 (+Peak trace) to display the readout.
TRACE1:DPSA:SELECT? might return 1, indicating that the readout is being displayed for Trace 1.

TRACe<x>:FVTime:DETection

Enables or queries the type of detection for the specified trace. The parameter <x> represents traces 1 to 4.

Conditions Measurement views: Frequency versus Time

Group Trace commands

Syntax TRACe<x>:FVTime:DETection { AVERAge | POSitive | NEGative | POSNegative | SAMPlE }
TRACe<x>:FVTime:DETection?

Arguments AVERAge displays the average data value for each pixel.
POSitive displays the maximum data value for each pixel.
NEGative displays the minimum data value for each pixel.
POSNegative displays the maximum and minimum data values for each pixel.
SAMPlE displays the first sample value received for each pixel.

Examples TRACe2:FVTime:DETection POSitive enables positive detection on Trace2.

TRACe<x>:PHVTime:DETection

Sets or queries the display detector (method to be used for decimating traces to fit the available horizontal space on screen). The number of horizontal pixels on screen is generally smaller than that of waveform data points. When actually displayed, the waveform data is therefore thinned out, according to the number of pixels, for being compressed.

Conditions	Measurement views: Phase versus Time
Group	Trace commands
Syntax	TRACe<x>:PHVTime:DETEction { AVERAge POSitive NEGative POSNegative SAMPlE } TRACe<x>:PHVTime:DETEction?
Arguments	AVERAge displays the average data value for each pixel. POSitive displays the maximum data value for each pixel. NEGative displays the minimum data value for each pixel. POSNegative displays the maximum and minimum data values for each pixel. SAMPlE displays the first sample value received for each pixel.
Examples	TRACe1:PHVTime:DETEction POSitive displays the maximum data value for each pixel.

TRACe<x>:PNOise:SElect

Selects the trace in the phase noise measurement. The query returns the currently selected trace.

The parameter <x> = 1 and 2.

Conditions	Measurement views: Phase noise
Group	Trace commands
Syntax	TRACe<x>:PNOise:SElect TRACe<x>:PNOise:SElect?
Arguments	None
Returns	0 (not selected) or 1 (selected).
Examples	TRACe2:PNOISE:SELECT selects Trace 2.

TRACe<x>:PNOise:SHOW

Determines whether to show or hide the specified trace in the phase noise view.

The parameter <x> = 1 and 2.

Conditions	Measurement views: Phase noise
Group	Trace commands
Syntax	TRACe<x>:PNOise:SHOW { OFF ON 0 1 } TRACe<x>:PNOise:SHOW?
Arguments	OFF or 0 hides the specified trace. ON or 1 shows the specified trace.
Examples	TRACE1:PNOISE:SHOW ON shows Trace 1 in the phase noise view.

TRACe<x>:PNOise:SMOothing:COUNT

Sets or queries the number of data points to take the moving average for smoothing the trace. This command is effective when [TRACe<x>:PNOise:SMOothing:ENABLE](#) is set to ON.

The parameter <x> = 1 and 2.

Conditions	Measurement views: Phase noise
Group	Trace commands
Syntax	TRACe<x>:PNOise:SMOothing:COUNT <number> TRACe<x>:PNOise:SMOothing:COUNT?
Arguments	<number>::=<NR1> specifies the number of data points to take the moving average for smoothing. Range: 3 to 50.
Examples	TRACE1:PNOISE:SMOOTHING:COUNT 16 sets the smoothing count to 16 for Trace 1.

TRACe<x>:PNOise:SMOothing:ENABle

Determines whether to enable or disable smoothing the specified trace in the phase noise view.

The parameter <x> = 1 and 2.

Conditions Measurement views: Phase noise

Group Trace commands

Syntax TRACe<x>:PNOise:SMOothing:ENABle { OFF | ON | 0 | 1 }
TRACe<x>:PNOise:SMOothing:ENABle?

Arguments OFF or 0 disables smoothing.
ON or 1 enables smoothing.

Examples TRACE1:PNOISE:SMOOTHING:ENABLE ON enables smoothing Trace 1 in the phase noise view.

TRACe<x>:PNOise:SMOothing:RESet (No Query Form)

Restarts the smoothing process, discarding accumulated data and resetting the counter. This command is effective when [TRACe<x>:PNOise:SMOothing:ENABle](#) is set to ON.

The parameter <x> = 1 and 2.

Conditions Measurement views: Phase noise

Group Trace commands

Syntax TRACe<x>:PNOise:SMOothing:RESet

Arguments None

Examples TRACE1:PNOISE:SMOOTHING:RESET restarts the smoothing process for Trace 1.

TRACe<x>:SPECTrum

Determines whether to show or hide the specified trace in the Spectrum view.

The parameter <x> = 1 to 5; All traces are valid.

Conditions	Measurement views: Spectrum
Group	Trace commands
Syntax	TRACe<x>:SPECTrum { OFF ON 0 1 } TRACe<x>:SPECTrum?
Arguments	OFF or 0 hides the specified trace. ON or 1 shows the specified trace. For Trace 5 (spectrogram), use the TRACe:SGRam:SElect:LINE command to select the number of line to send to the spectrum display.
Examples	TRACE1:SPECTRUM ON shows Trace 1 in the Spectrum Analyzer view.

TRACe<x>:SPECTrum:AVERAge:COUNT

Sets or queries the number of traces to combine. This command is effective when [TRACe<x>:SPECTrum:FUNCTION](#) is AVERAge, MAXHold or MINHold.

The parameter <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Conditions	Measurement views: Spectrum
Group	Trace commands
Syntax	TRACe<x>:SPECTrum:AVERAge:COUNT <number> TRACe<x>:SPECTrum:AVERAge:COUNT?
Arguments	<number> ::= <NR1> specifies the number of traces to combine for averaging. Range: 1 to 10000.

Examples TRACE1:SPECTRUM:AVERAGE:COUNT 64 sets the average count to 64 for Trace 1.

TRACe<x>:SPECTrum:AVERAge:RESet (No Query Form)

Clears average data and counter, and restarts the average process for the specified trace in the Spectrum view. This command is effective when TRACe<x>:SPECTrum:FUNCTion is set to AVERAge, MAXHold or MINHold.

The parameter <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Conditions Measurement views: Spectrum

Group Trace commands

Syntax TRACe<x>:SPECTrum:AVERAge:RESet

Arguments None

Examples TRACE1:SPECTRUM:AVERAGE:RESET clears average data and counter, and restarts the average process for Trace 1.

TRACe<x>:SPECTrum:COUNT

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Spectrum measurement. This command is effective when TRACe<x>:SPECTrum:FUNCTion is set to MAXHold or MINHold and INITiate:CONTInuous is set to OFF.

The parameter <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Conditions Measurement views: Spectrum

Group Trace commands

Syntax TRACe<x>:SPECTrum:COUNT <number>
TRACe<x>:SPECTrum:COUNT?

Arguments `<number>::=<NR1>` specifies the count for Max/Min Hold. Range: 1 to 10000.

Examples `TRACE1:SPECTRUM:COUNT 32` sets the count to 32 for Trace 1.

TRACe<x>:SPECTrum:COUNT:ENABLE

Determines whether to enable or disable the count for the Max or Min Hold trace in the Spectrum view. This command is effective when [TRACe<x>:SPECTrum:FUNCTION](#) is set to MAXHold or MINHold.

The parameter `<x>` = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Conditions Measurement views: Spectrum

Group Trace commands

Syntax `TRACe<x>:SPECTrum:COUNT:ENABLE { OFF | ON | 0 | 1 }`
`TRACe<x>:SPECTrum:COUNT:ENABLE?`

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
 ON or 1 enables the count for the Max/Min Hold trace.

Examples `TRACE1:SPECTRUM:COUNT:ENABLE ON` enables the Max/Min Hold count for Trace 1.

TRACe<x>:SPECTrum:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process for the specified trace in the Spectrum view. This command is effective when [TRACe<x>:SPECTrum:FUNCTION](#) is set to MAXHold or MINHold.

The parameter `<x>` = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Conditions Measurement views: Spectrum

Group Trace commands

Syntax TRACE<x>:SPECTrum:COUNT:RESet

Arguments None

Examples TRACE1:SPECTRUM:COUNT:RESET clears the Max/Min Hold data and counter, and restarts the process for Trace 1.

TRACe<x>:SPECtrum:DETection

Sets or queries the display detector (method to be used for decimating traces to fit the available horizontal space on screen). The number of horizontal pixels on screen is generally smaller than that of waveform data points. When actually displayed, the waveform data is therefore thinned out, according to the number of pixels, for being compressed.

The parameter <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Conditions Measurement views: Spectrum

Group Trace commands

Syntax TRACe<x>:SPECtrum:DETection { AVERAge | POSitive | NEGative
| CAVERage | CPEak | QUASipeak | SAMPlE}
TRACe<x>:SPECtrum:DETection?

Arguments AVERAge displays the average data value for each pixel.
POSitive displays the maximum data value for each pixel.
NEGative displays the minimum data value for each pixel.
CAVERage displays the CISPR average value for each pixel.
CPEak displays the CISPR peak value for each pixel.
QUASipeak displays the quasi-peak value for each pixel.
SAMPlE displays the most recent sample value for each pixel.

Examples TRACE1:SPECTRUM:DETECTION POSitive displays the maximum data value for each pixel on Trace 1.

TRACe<x>:SPECTrum:FREEze

Determines whether or not to freeze the display of the specified trace in the Spectrum view.

The parameter <x> = 1 to 5; All traces are valid.

Conditions	Measurement views: Spectrum
Group	Trace commands
Syntax	TRACe<x>:SPECTrum:FREEze { OFF ON 0 1 } TRACe<x>:SPECTrum:FREEze?
Arguments	OFF or 0 updates the display of the specified trace normally. ON or 1 stops updating the display of the specified trace.
Examples	TRACE1:SPECTRUM:FREEZE ON freezes Trace 1 in the Spectrum Analysis display.

TRACe<x>:SPECTrum:FUNCTION

Sets or queries the function for the specified trace in the Spectrum view.

The parameter <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Conditions	Measurement views: Spectrum
Group	Trace commands
Syntax	TRACe<x>:SPECTrum:FUNCTION { NONE AVERAGE MAXHOLD MINHOLD } TRACe<x>:SPECTrum:FUNCTION?
Arguments	NONE selects the normal spectrum display. AVERAGE selects the Average display that indicates the average signal level at each frequency point.

MAXHold selects the Max Hold display that indicates the maximum signal level at each frequency point.

MINHold selects the Min Hold display that indicates the minimum signal level at each frequency point.

Examples `TRACE1:SPECTRUM:FUNCTION MAXHold` selects Max Hold for Trace 1 in the Spectrum view.

TRACe<x>:SPECtrum:LEFToperand

Sets or queries the left operand for the math trace (Trace 4) in the Spectrum view.

The parameter <x> = 4; Only Trace 4 (math trace) is valid.

Conditions Measurement views: Spectrum

Group Trace commands

Syntax `TRACe<x>:SPECtrum:LEFToperand { TRACE1 | TRACE2 | TRACE3 }`
`TRACe<x>:SPECtrum:LEFToperand?`

Related Commands [TRACe<x>:SPECtrum:RIGHToperand](#)

Arguments `TRACE1` selects Trace 1 as the left operand for the math trace.

`TRACE2` selects Trace 2 as the left operand for the math trace.

`TRACE3` selects Trace 3 as the left operand for the math trace.

Examples `TRACE4:SPECTRUM:LEFTOPERAND TRACE1` selects Trace 1 as the left operand for the math trace.

TRACe<x>:SPECtrum:RIGHToperand

Sets or queries the right operand for the math trace (Trace 4) in the Spectrum view.

The parameter <x> = 4; Only Trace 4 (math trace) is valid.

Conditions Measurement views: Spectrum

Group	Trace commands
Syntax	TRACe<x>:SPECTrum:RIGHToperand { TRACE1 TRACE2 TRACE3 } TRACe<x>:SPECTrum:RIGHToperand?
Related Commands	TRACe<x>:SPECTrum:LEFToperand
Arguments	TRACE1 selects Trace 1 as the right operand for the math trace. TRACE2 selects Trace 2 as the right operand for the math trace. TRACE3 selects Trace 3 as the right operand for the math trace.
Examples	TRACE4:SPECTRUM:RIGHTOPERAND TRACE1 selects Trace 1 as the right operand for the math trace.

TRACe<x>:SPECTrum:SElect

Sets or queries the trace to display the readout at the upper left of the Spectrum view.

The parameter <x> = 1 to 5; All traces are valid.

NOTE. TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.

Conditions	Measurement views: Spectrum
Group	Trace commands
Syntax	TRACe<x>:SPECTrum:SElect TRACe<x>:SPECTrum:SElect?
Arguments	None
Returns	{ 0 1 } 0 indicates that the readout is not being displayed for the specified trace. 1 indicates that the readout is being displayed for the specified trace.

Examples TRACE1:SPECTRUM:SELECT selects Trace 1 to display the readout.
 TRACE1:SPECTRUM:SELECT? might return 1, indicating that the readout is being displayed for Trace 1.

*TRG (No Query Form)

Generates a trigger. It produces the same effect as the Force Trigger button on the Trigger control panel. This command is valid when the trigger mode is Triggered.

Conditions Measurement views: All

Group IEEE common commands

Syntax *TRG

Related Commands [TRIGger\[:SEQUence\]:TIME:QUALified:TIME<x>](#)

Arguments None

Examples *TRG generates a trigger.

TRIGger:DPSA:SHOW:FRAMES

Determines when to show frames in the swept acquisition mode. Show frames continuously when ON or show only triggered frames when OFF.

Conditions Measurement views: All
 Option 200 only

Group Trigger commands

Syntax TRIGger:DPSA:SHOW:FRAMES { OFF | ON | 0 | 1 }
 TRIGger:DPSA:SHOW:FRAMES?

- Arguments** OFF or 0 shows only triggered frames.
ON or 1 shows frames continuously.
- Examples** TRIGGER:DPSA:SHOW:FRAMES ON shows frames continuously.

TRIGGER:MASK:NEW (No Query Form)

Loads a new frequency mask.

- Conditions** Measurement views: All
- Group** Trigger commands
- Syntax** TRIGGER:MASK:NEW <freq(1)>,<amp1(1)>,<freq(2)>,<amp1(2)>,
...,<freq(n)>,<amp1(n)> (n = 500 maximum)
- Arguments** <freq(n)>,<amp1(n)> is a frequency (Hz) and amplitude (dBm) pair to specify a point of the mask. Up to 500 pairs can be specified with zero frequency being the center screen. The mask is visible in the spectrum view with the following trigger conditions
- Trigger mode: Triggered (TRIGGER[:SEQUENCE]:TIME:QUALIFIED:TIME<x> is set to ON or 1.)
 - Trigger type: Frequency Mask (TRIGGER[:SEQUENCE]:EVENT:INPUT:TYPE is set to FMASK.)
- Examples** TRIGGER:MASK:NEW -8E6,-80,0,-10,8E6,-80 loads the mask with the points A (-8 MHz, -80 dBm), B (0 Hz, -10 dBm), and C (8 MHz, -80 dBm), as shown in the following figure.

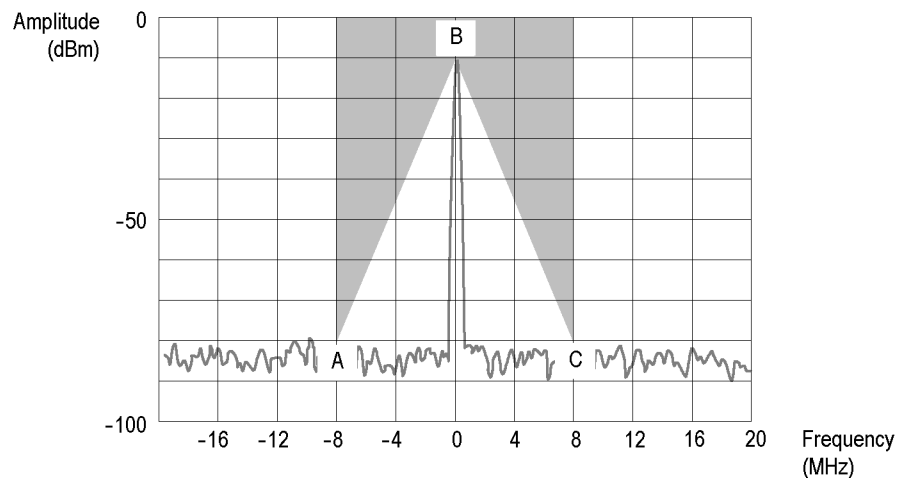


Figure 2-6: Trigger mask setting example

TRIGger:MASK:NEW:AUTO (No Query Form)

Draws a new frequency mask automatically based on a reference trace.

Conditions Measurement views: All

Group Trigger commands

Syntax TRIGger:MASK:NEW:AUTO
 <meas_ID>, <trace_ID>, <x_margin>, <y_margin>

Arguments <meas_ID>::=<string> specifies the measurement view.

<trace_ID> specifies the reference trace.

The values of <meas_ID> and <trace_ID> are listed in the following table for each possible measurement view.

<x_margin>::=<NRf> specifies the X margin (horizontal offset from the reference trace) in Hz.

<y_margin>::=<NRf> specifies the Y margin (vertical offset from the reference trace) in dB.

Measurement view	<meas_ID>	<trace_ID>
Spectrum	"specan"	TRACE1 (Trace 1), TRACE2 (Trace 2), TRACE3 (Trace 3), TRACE4 (Math trace), TRACE5 (Spectrogram trace)
DPX spectrum	"dpsa"	TRACE1 (+Peak trace), TRACE2 (-Peak trace), TRACE3 (Avg trace), TRACE4 (Math trace)
Channel power and ACPR	"acpr"	TRACE1 (Trace 1)
MCPR	"mcpr"	TRACE1 (Trace 1)
OBW	"obw"	TRACE1 (Trace 1)

Examples TRIGGER:MASK:NEW:AUTO "specan", TRACE1, 2E+6, 15 draws a new frequency mask automatically in the Spectrum view based on Trace 1 with the horizontal margin of 2 MHz and the vertical margin of 15 dB.

TRIGger:MASK:OPEN (No Query Form)

Opens a trigger mask with a specified file. To save a trigger mask, use the [TRIGger:MASK:SAVE](#) command.

Conditions Measurement views: All

Group Trigger commands

Syntax TRIGger:MASK:OPEN <file_name>

Arguments <file_name>::=<string> specifies the trigger mask file to open. The file extension is .msk. You can omit the extension.

For the directory of file, refer to *Specifying the File* (See page 2-47.)

Examples TRIGGER:MASK:OPEN "C:\My Documents\Mask1" opens the trigger mask with the *Mask1* file in the *My Documents* directory.

TRIGger:MASK:SAVE (No Query Form)

Saves the current trigger mask to a specified file. To open the trigger mask, use the [TRIGger:MASK:OPEN](#) command.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger:MASK:SAVE <file_name>
Arguments	<file_name>::=<string> specifies the file to save the trigger mask. The file extension is .msk. You can omit the extension. For the directory of file, refer to <i>Specifying the File</i> (See page 2-47.)
Examples	TRIGGER:MASK:SAVE "C:\My Documents\Mask1" saves the trigger mask to the <i>Mask1</i> file in the <i>My Documents</i> directory.

TRIGger[:SEQUence]:ADVanced:HOLDoff

Sets or queries the trigger holdoff time which prevents triggers until there have been no trigger events for at least the specified holdoff period.

Conditions	Measurement views: All Option 200 only
Group	Trigger commands
Syntax	TRIGger[:SEQUence]:ADVanced:HOLDoff <value> TRIGger[:SEQUence]:ADVanced:HOLDoff?
Arguments	<value>::=<NRf> specifies the trigger holdoff time. Range: 20 ns to 10 s.
Examples	TRIGger[:SEQUence]:ADVanced:HOLDoff 1.5us sets the trigger holdoff time to 1.5 μ s.

TRIGger[:SEquence]:ADVanced:HOLDoff:ENABLE

Enables or queries the status of the Advanced Trigger Holdoff function.

Conditions	Measurement views: All Option 200 only
Group	Trigger commands
Syntax	TRIGger[:SEquence]:ADVanced:HOLDoff:ENABle { OFF ON 0 1 } TRIGger[:SEquence]:ADVanced:HOLDoff:ENABle?
Arguments	OFF or 0 does not trigger based on the advanced trigger holdoff settings. ON or 1 enables triggering based on the advanced trigger holdoff settings.
Examples	TRIGger:ADVanced:HOLDoff:ENABle ON enables triggering based on the advanced trigger holdoff settings.

TRIGger[:SEquence]:ADVanced:SWEEp:MODE

Determines whether or not to trigger each segment in the swept acquisition mode.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEquence]:ADVanced:SWEEp:MODE { OFF ON 0 1 } TRIGger[:SEquence]:ADVanced:SWEEp:MODE?
Arguments	OFF or 0 does not trigger each segment in the swept acquisition mode. ON or 1 triggers each segment in the swept acquisition mode.
Examples	TRIGGER:SEQUENCE:ADVANCED:SWEEP:MODE ON triggers each segment in the swept acquisition mode.

TRIGger[:SEQuence]:ADVanced:SWEPT:SEGMENT:ENABLE

Determines whether or not to set the spectrum analyzer to wait for a trigger for each acquisition in a swept spectrum or other measurement requiring multiple acquisitions worth of span.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:ADVanced:SWEPT:SEGMENT:ENABle { OFF ON 0 1 } TRIGger[:SEQuence]:ADVanced:SWEPT:SEGMENT:ENABle?
Arguments	OFF or 0 does not trigger each segment in the swept acquisition mode. ON or 1 triggers each segment in the swept acquisition mode.
Examples	TRIGger[:SEQuence]:ADVanced:SWEPT:SEGMENT:ENABle ON waits for a trigger for each acquisition in a swept spectrum or other measurement requiring multiple acquisitions worth of span.

TRIGger[:SEQuence]:EVENT:EXTFront:IMPedance

Sets or queries the impedance of the external trigger input on the front panel.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:EVENT:EXTFront:IMPedance { OHM50 OHM5K } TRIGger[:SEQuence]:EVENT:EXTFront:IMPedance?
Arguments	OHM50 selects 50 Ω impedance. OHM5K selects 5 k Ω impedance.
Examples	TRIGGER:SEQUENCE:EVENT:EXTFRONT:IMPEDANCE OHM50 selects 50 Ω impedance for the external trigger input on the front panel.

TRIGger[:SEQuence]:EVENT:EXTFront:LEVel

Sets or queries the trigger level at the external trigger input on the front panel.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:EVENT:EXTFront:LEVel <value> TRIGger[:SEQuence]:EVENT:EXTFront:LEVel?
Arguments	<value> ::= <Nrf> specifies the trigger level. Range: -2.5 to +2.5 V.
Examples	TRIGGER:SEQUENCE:EVENT:EXTFRONT:LEVEL 1.5 sets the trigger level to 1.5 V at the external trigger input on the front panel.

TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe

Sets or queries the trigger slope of the external trigger input on the front panel.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe { RISE FALL } TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe?
Arguments	RISE causes the trigger event on the rising edge. FALL causes the trigger event on the falling edge.
Examples	TRIGGER:SEQUENCE:EVENT:EXTFRONT:SLOPE RISE causes the trigger event on the rising edge of the external input signal.

TRIGger[:SEQuence]:EVENT:EXTRear:SLOPe

Sets or queries the trigger slope of the external trigger input on the rear panel. The trigger level is fixed to the TTL threshold.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:EVENT:EXTREar:SLOPe { RISE FALL } TRIGger[:SEQuence]:EVENT:EXTREar:SLOPe?
Arguments	RISe causes the trigger event on the rising edge. FALL causes the trigger event on the falling edge.
Examples	TRIGGER:SEQUENCE:EVENT:EXTREAR:SLOPE RISE causes the trigger event on the rising edge of the external input signal.

TRIGger[:SEQuence]:EVENT:GATed

Sets or queries the positive or negative logic for the gated trigger input on the rear panel.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:EVENT:GATed { HIGH LOW } TRIGger[:SEQuence]:EVENT:GATed?
Arguments	HIGH specifies that the gated trigger input is high active. LOW specifies that the gated trigger input is low active.
Examples	TRIGGER:SEQUENCE:EVENT:GATED HIGH specifies that the gated trigger input is high active.

TRIGger[:SEQuence]:EVENT:INPut:DDENsity:AMPLitude

Sets or queries the center vertical level for the density trigger region of the RF input DPX bitmap display.

Conditions	Measurement views: DPX bitmap
-------------------	-------------------------------

Option 200 only

Group Trigger commands

Syntax TRIGger[:SEquence]:EVENT:INPut:DDENsity:AMPLitude <value>
TRIGger[:SEquence]:EVENT:INPut:DDENsity:AMPLitude?

Related Commands [TRIGger\[:SEquence\]:EVENT:INPut:DDENsity:AMPLitude:TOLerance](#)

Arguments <value>::=<Nrf> specifies the vertical center of the trigger region in dBm. Range: 0 to 200 dBm.

Examples TRIGger[:SEquence]:EVENT:INPut:DDENsity:AMPLitude 100dBm sets the center level to 100 dBm for the density trigger region.

TRIGger[:SEquence]:EVENT:INPut:DDENsity:AMPLitude:TOLerance

Sets or queries the positive and negative extensions of the density trigger region from the center vertical level. The density trigger region is defined for the DPX bitmap display.

Conditions Measurement views: DPX bitmap

Option 200 only

Group Trigger commands

Syntax TRIGger[:SEquence]:EVENT:INPut:DDENsity:AMPLitude:TOLerance <value>
TRIGger[:SEquence]:EVENT:INPut:DDENsity:AMPLitude:TOLerance?

Related Commands [TRIGger\[:SEquence\]:EVENT:INPut:DDENsity:FREQuency:TOLerance](#)

Arguments <value>::=<Nrf> specifies an absolute amplitude value for the positive and negative limits of the density trigger region in dBm. Range: within the defined measurement box.

Examples TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:AMPLITUDE:TOLERANCE 50dBm sets the positive limit 50 dBm above the AMPLITUDE level and the negative limit 50 dBm below the AMPLITUDE level.

TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:FREQUENCY

Sets or queries the center horizontal level for the density trigger region of the RF input DPX bitmap display.

Conditions Measurement views: DPX bitmap
Option 200 only

Group Trigger commands

Syntax TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:FREQUENCY <value>
TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:FREQUENCY?

Related Commands

Arguments <value>::=<NRF> specifies the horizontal center of the trigger region. Range: within the defined measurement box.

Examples TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:FREQUENCY 1.82GHz sets the center horizontal level to 1.82 GHz for the density trigger region.

TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:FREQUENCY:TOLERANCE

Sets or queries the left and right extensions of the density trigger region from the center horizontal level. The density trigger region is defined for the DPX bitmap display.

Conditions Measurement views: DPX bitmap
Option 200 only

Group Trigger commands

Syntax TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:FREQUENCY:TOLERANCE <value>
TRIGGER[:SEQUENCE]:EVENT:INPUT:DDENSITY:FREQUENCY:TOLERANCE?

Related Commands

Arguments `<value>::=<Nrf>` specifies an absolute frequency value for the left and right limits from the center frequency of the density trigger region. Range: within the defined measurement box.

Examples `TRIGger[:SEquence]:EVENT:INPut:DDENsity:FREQuency:TOLerance 0.2GHZ`, for a center frequency of 1.82 GHz, sets the left horizontal limit to 1.62 GHz and the right horizontal limit to 2.02 GHz for the density trigger region.

TRIGger[:SEquence]:EVENT:INPut:DDENsity:THReshold

Sets or queries the DPX Density threshold that defines a trigger event for the density trigger region of the DPX bitmap display. The DPX Density must be higher or lower (specified by the Density selection) than this value to define a trigger event.

Conditions Measurement views: DPX bitmap
Option 200 only

Group Trigger commands

Syntax `TRIGger[:SEquence]:EVENT:INPut:DDENsity:THReshold <value>`
`TRIGger[:SEquence]:EVENT:INPut:DDENsity:THReshold?`

Related Commands

Arguments `<value>::=<Nrf>` specifies the DPX Density threshold as a percentage (%). Range: within the defined measurement box.

Examples `TRIGger[:SEquence]:EVENT:INPut:DDENsity:THReshold 2` sets the DPX Density threshold to 2 % for the density trigger.

TRIGger[:SEquence]:EVENT:INPut:DDENsity:VIOLation

Sets or queries whether a density value higher or lower than the THReshold value defines a trigger event for the density trigger region of the DPX bitmap display.

Conditions Measurement views: DPX bitmap
Option 200 only

Group	Trigger commands
Syntax	<pre>TRIGger[:SEquence]:EVENT:INPut:DDENsity:VIOLation { HIGHer Lower } TRIGger[:SEquence]:EVENT:INPut:DDENsity:VIOLation?</pre>
Related Commands	TRIGger[:SEquence]:EVENT:INPut:DDENsity:THReshold
Arguments	<p>HIGHer a DPX density value above the THReshold value defines the trigger event.</p> <p>Lower a DPX Density value below the THReshold value defines the trigger event.</p>
Examples	<pre>TRIGger:EVENT:INPut:DDENsity:VIOLation LOWER sets the DPX Density VIOLATION to trigger when the probability of occurrence is lower than the THRESHOLD percentage.</pre>

TRIGger[:SEquence]:EVENT:INPut:FMASK:{BANDwidth|BWIDth}[:RESolution]

Sets or queries the Resolution Bandwidth value to be used in the spectrum view for the frequency mask trigger.

Conditions	<p>Measurement views: All</p> <p>Option 200 only</p>
Group	Trigger commands
Syntax	<pre>TRIGger[:SEquence]:EVENT:INPut:FMASK:{BANDwidth BWIDth}[: RESolution] <value> TRIGger[:SEquence]:EVENT:INPut:FMASK:{BANDwidth BWIDth}[: RESolution]?</pre>
Arguments	<p><value>::=<NRF> specifies the resolution bandwidth for Frequency Mask triggering. Range: .</p>
Examples	<pre>TRIGger[:SEquence]:EVENT:INPut:FMASK:Bandwidth 300kHz sets the resolution bandwidth to 300 kHz.</pre>

TRIGger[:SEquence]:EVENT:INPut:FMASK:BANDwidth|BWIDth[:RESolution]:ACTual? (Query Only)

Queries current setting for the Resolution Bandwidth value used in the spectrum view for the frequency mask trigger.

Conditions Measurement views: All
Option 200 only

Group Trigger commands

Syntax TRIGger[:SEquence]:EVENT:INPut:FMASK:BANDwidth|BWIDth[:RESolution]:ACTual?

Arguments None.

Examples TRIGger:EVENT:INPut:FMASK:BWIDth:ACTUAL? returns the resolution bandwidth value.

TRIGger[:SEquence]:EVENT:INPut:FMASK:BANDwidth|BWIDth[:RESolution]:AUTO

Sets or queries whether to automatically set the Resolution Bandwidth value used in the spectrum view for the frequency mask trigger.

Conditions Measurement views: All
Option 200 only

Group Trigger commands

Syntax TRIGger[:SEquence]:EVENT:INPut:FMASK:BANDwidth|BWIDth[:RESolution]:AUTO { OFF | ON | 0 | 1 }
TRIGger[:SEquence]:EVENT:INPut:FMASK:BANDwidth|BWIDth[:RESolution]:AUTO?

Arguments OFF or 0 sets the resolution bandwidth manually with the command TRIGger[:SEquence]:EVENT:INPut:FMASK: {BANDwidth|BWIDth}[:RESolution].

ON or 1 sets the resolution bandwidth automatically.

Examples TRIGGER:EVENT:INPUT:FMASK:BWIDTh:AUTO ON sets the resolution bandwidth automatically.

TRIGGER[:SEQUENCE]:EVENT:INPUT:FMASK:VIOLATION

Sets or queries when the analyzer triggers in the frequency mask trigger.

Conditions Measurement views: All

Group Trigger commands

Syntax TRIGGER[:SEQUENCE]:EVENT:INPUT:FMASK:VIOLATION { T | F | TF | FT | TFT | FTF }
 TRIGGER[:SEQUENCE]:EVENT:INPUT:FMASK:VIOLATION?

Arguments The following table lists the arguments which represent the trigger violations.

Table 2-46: Trigger violations

Violation	Description
T	Only one state is required to initiate a trigger event. The signal has at least one data point inside the mask. The trigger event occurs at the first point that appears inside the mask. A trigger event could occur on the first acquisition.
F	Only one state change is required to initiate a trigger event. The signal has at least one data point outside the mask. The trigger event occurs at the first point that appears outside the mask. A trigger event could occur on the first acquisition.
TF	Two states are required to initiate a trigger event. The signal must be inside the mask and then passes out of the mask. The trigger event occurs at the first transition where the signal passes out of the mask.
FT	Two states are required to initiate a trigger event. The signal must be outside the mask and then passes into the mask. The trigger event occurs at the first transition where the signal passes into the mask.
TFT	Three states are required to initiate a trigger event. The signal starts inside the mask and then passes out of the mask. Next, the signal must pass into the mask. The trigger event occurs at the second transition where the signal passes back into the mask.
FTF	Three states are required to initiate a trigger event. The signal starts outside the mask and then passes into the mask. Next, the signal must pass back outside the mask. The trigger event occurs at the second transition where the signal passes back out of the mask.

Examples TRIGGER:SEQUENCE:EVENT:INPUT:FMASK:VIOLATION TF specifies that the analyzer will trigger when the signal has crossed into the mask and then outside of the mask.

TRIGger[:SEQuence]:EVENT:INPut:LEVel

Sets or queries the trigger level for the RF input level trigger.

Conditions Measurement views: All

Group Trigger commands

Syntax TRIGger[:SEQuence]:EVENT:INPut:LEVel <value>
TRIGger[:SEQuence]:EVENT:INPut:LEVel?

Arguments <value> ::= <Nrf> specifies the trigger level. Range: -170 to +50 dBm.

Examples TRIGGER:SEQUENCE:EVENT:INPUT:LEVEL -10 sets the trigger level to -10 dBm for the RF input level trigger.

TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe

Sets or queries the Runt trigger for a positive or negative going pulse.

Conditions Measurement views: All
Option 200 only

Group Trigger commands

Syntax TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe { POSitive |
NEGative }
TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe?

Arguments POSitive causes the trigger event on a positive runt pulse.
NEGative causes the trigger event on a negative runt pulse.

Examples TRIGger:EVENT:INPut:RUNT:PULSE POSitive causes the trigger event on a positive pulse.

TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe:HIGh:LEVel

Sets or queries the upper level (first threshold) to qualify a Runt trigger.

Conditions Measurement views: All
Option 200 only

Group Trigger commands

Syntax TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe:HIGh:LEVel <value>
TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe:HIGh:LEVel?

Arguments <value>::=<Nrf> sets the upper vertical level for a runt pulse in dBm.

Examples TRIGger:EVENT:INPut:RUNT:PULSE 300 causes the trigger event when the leading edge of a pulse crosses the 300 dBm level.

TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe:LOW:LEVel

Sets or queries the lower level (second threshold) to qualify a Runt trigger.

Conditions Measurement views: All
Option 200 only

Group Trigger commands

Syntax TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe:LOW:LEVel <value>
TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULSe:LOW:LEVel?

Arguments <value>::=<Nrf> sets the lower vertical level for a runt pulse in dBm.

Examples TRIGger:EVENT:INPut:RUNT:PULSE 3 causes the trigger event when the following edge of a pulse crosses the 3 dBm level.

TRIGger[:SEQuence]:EVENT:INPut:SLOPe

Sets or queries the trigger slope for the RF input level trigger.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:EVENT:INPut:SLOPe { RISE FALL } TRIGger[:SEQuence]:EVENT:INPut:SLOPe?
Arguments	RISE causes the trigger event on the rising edge. FALL causes the trigger event on the falling edge.
Examples	TRIGGER:SEQUENCE:EVENT:INPUT:SLOPE RISE causes the trigger event on the rising edge of the RF input signal.

TRIGger[:SEQuence]:EVENT:INPut:TDBWidth

Sets or queries the time-domain bandwidth for the RF input power trigger. This command is effective when [TRIGger\[:SEQuence\]:EVENT:INPut:TDBWidth:STATe](#) is ON.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:EVENT:INPut:TDBWidth <value> TRIGger[:SEQuence]:EVENT:INPut:TDBWidth?
Arguments	<value> ::= <NRf> specifies the time-domain bandwidth. Range: 1 Hz to 60 MHz.
Examples	TRIGGER:SEQUENCE:EVENT:INPUT:TDBWIDTH 5MHZ sets the time-domain bandwidth to 5 MHz for the RF input power trigger.

TRIGger[:SEquence]:EVENT:INPut:TDBWidth:ACTual? (Query Only)

Queries the actual time-domain bandwidth for the RF input power trigger.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEquence]:EVENT:INPut:TDBWidth:ACTual?
Related Commands	TRIGger[:SEquence]:EVENT:INPut:TDBWidth
Arguments	None
Returns	<NRF> Actual time-domain bandwidth.
Examples	TRIGGER:SEQUENCE:EVENT:INPUT:TDBWIDTH:ACTUAL? might return 1.000E+6, indicating that the actual time-domain bandwidth is 1 MHz.

TRIGger[:SEquence]:EVENT:INPut:TDBWidth:STATE

Determines whether to set the time-domain bandwidth automatically or manually for the RF input power trigger.

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEquence]:EVENT:INPut:TDBWidth:STATE { OFF ON 0 1 } TRIGger[:SEquence]:EVENT:INPut:TDBWidth:STATE?
Arguments	OFF or 0 sets the time-domain bandwidth automatically. ON or 1 sets the time-domain bandwidth manually using the TRIGger[:SEquence]:EVENT:INPut:TDBWidth command.

Examples TRIGGER:SEQUENCE:EVENT:INPUT:TDBWIDTH:STATE OFF sets the time-domain bandwidth automatically.

TRIGger[:SEQuence]:EVENT:INPut:TYPE

Sets or queries the trigger type for the source of RF input.

Conditions Measurement views: All

Arguments DDENSITY and RUNT are Option 200 only

Group Trigger commands

Syntax TRIGger[:SEQuence]:EVENT:INPut:TYPE { POWER | FMASK |
DDENSITY | RUNT }
TRIGger[:SEQuence]:EVENT:INPut:TYPE?

Arguments POWER uses the power level for triggering.
FMASK uses the frequency mask for triggering.
DDENSITY uses the density mask for triggering.
RUNT uses the runt mask for triggering.

Examples TRIGGER:SEQUENCE:EVENT:INPUT:TYPE FMASK uses the frequency mask for triggering.

TRIGger[:SEQuence]:EVENT:SOURce

Sets or queries the trigger event source.

Conditions Measurement views: All

Group Trigger commands

Syntax TRIGger[:SEQuence]:EVENT:SOURce { INPut | EXTFront | EXTRear
| EXTGated | LINE }
TRIGger[:SEQuence]:EVENT:SOURce?

Arguments The following table lists the arguments.

Table 2-47: Trigger event source

Argument	Source
INPut	RF input
EXTFront	Trigger in (front)
EXTRear	Trigger in (rear)
EXTGated	Gate in
LINe	AC line

Examples TRIGGER:SEQUENCE:EVENT:SOURCE INPut specifies the trigger event source as the RF input.

TRIGger[:SEQuence]:FORCed

Determines whether or not to cause a manual trigger if the acquisition is armed, ready and waiting for a trigger. This command is valid when [TRIGger\[:SEQuence\]:TIME:QUALified:TIME<x>](#) is set to On (the trigger mode is Triggered).

Conditions Measurement views: All

Group Trigger commands

Syntax TRIGger[:SEQuence]:FORCed { OFF | ON | 0 | 1 }
TRIGger[:SEQuence]:FORCed?

Arguments OFF or 0 does not cause a manual trigger.
ON or 1 causes a manual trigger.

Examples TRIGGER:SEQUENCE:FORCED ON causes a manual trigger if the acquisition is armed, ready and waiting for a trigger.

TRIGger[:SEQuence]:IMMediate (No Query Form)

Causes a trigger immediately, skipping the event detection and delay. This command is valid when [TRIGger\[:SEQuence\]:TIME:QUALified:TIME<x>](#) is set to On (the trigger mode is Triggered).

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:IMMediate
Arguments	None
Examples	TRIGGER:SEQUENCE:IMMEDIATE causes a trigger immediately, skipping the event detection and delay.

TRIGger[:SEQuence]:STATus

Sets or queries the trigger mode (Free Run or Triggered).

Conditions	Measurement views: All
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:STATus { OFF ON 0 1 } TRIGger[:SEQuence]:STATus?
Arguments	OFF or 0 selects the free-run mode. ON or 1 selects the triggered mode.
Examples	TRIGGER:SEQUENCE:STATUS ON selects the triggered mode.

TRIGger[:SEQuence]:TIME:DELay

Sets or queries the trigger delay time which occurs after recognizing an event but before actually declaring the trigger.

Conditions	Measurement views: All
Group	Trigger commands

Syntax TRIGger[:SEquence]:TIME:DElay <value>
TRIGger[:SEquence]:TIME:DElay?

Arguments <value>::=<NRF> specifies the trigger delay time. Range: 0 to 60 s.

Examples TRIGGER:SEQUENCE:TIME:DELAY 1.5 sets the trigger delay time to 1.5 s.

TRIGger[:SEquence]:TIME:POSition

Sets or queries the position of the trigger event within the acquisition record.

Conditions Measurement views: All

Group Trigger commands

Syntax TRIGger[:SEquence]:TIME:POSition <value>
TRIGger[:SEquence]:TIME:POSition?

Arguments <value>::=<NRF> specifies the trigger position. Range: 1% to 99%.

Examples TRIGGER:SEQUENCE:TIME:POSITION 20 sets the trigger position to 20% of the acquisition record.

TRIGger[:SEquence]:TIME:QUALified

Sets or queries the timing qualification setting for triggers. Trigger events that do not meet the timing qualifications are ignored.

Conditions Measurement views: All
Option 200 only

Group Trigger commands

Syntax TRIGger[:SEquence]:TIME:QUALified { SHORTer | LONGer |
INSide | OUTSide | NONE }
TRIGger[:SEquence]:TIME:QUALified?

Related Commands

Arguments	<p>SHORTer the length of the trigger event is shorter than the time specified by the TRIGger:TIME:QUALified:TIME1 setting.</p> <p>LONGer the length of the trigger event is longer than the time specified by the TRIGger:TIME:QUALified:TIME1 setting.</p> <p>INSide the length of the trigger event is longer than the time TRIGger:TIME:QUALified:TIME1 setting and shorter than the TRIGger:TIME:QUALified:TIME2 setting.</p> <p>OUTSide the length of the trigger event is shorter than the time TRIGger:TIME:QUALified:TIME1 setting or longer than the TRIGger:QUALified:TIME2 setting.</p>
Examples	TRIGger:SEQuence:TIME:QUALified SHORTer the length of the trigger event is shorter than the time specified by the TRIGger:TIME:DELAY setting

TRIGger[:SEQuence]:TIME:QUALified:TIME<x>

Sets or queries the Time1 and Time2 parameters for time qualified triggering. Time1 is the shorter or first time, and Time2 is the second or later time for the qualifying period. Each TIME<x> must be set with a separate command.

Conditions	Measurement views: All Option 200 only
Group	Trigger commands
Syntax	TRIGger[:SEQuence]:TIME:QUALified:TIME<x> <value>

Related Commands [TRIGger\[:SEQuence\]:TIME:QUALified](#)

Arguments	<value> ::= <NRf> the length of the trigger time for TIME1 or TIME2. Range: 0 s to 28 s.
Examples	TRIGger:TIME:QUALified:TIME1 55us sets the TIME1 trigger point at 55 us after the trigger event.

UNIT:POWer

Sets or queries the fundamental unit of power. This command is equivalent to [\[SENSe\]:POWer:UNITs](#).

Conditions	Measurement views: All
Group	Unit commands
Syntax	UNIT:POWer { DBM DBV VOLTs WATTs DBUW DBW DBUV DBMV DBUA DBUV_M DBUA_M AMPS } UNIT:POWer?
Arguments	The following table lists the arguments.

Table 2-48: Power units

Argument	Power unit
DBM	dBm
DBV	dBV
VOLTs	Volts
WATTs	Watts
DBUW	dB μ W
DBW	dBW
DBUV	dB μ V
DBMV	dBmV
DBUA	dB μ A
DBUV_M	dB μ V/m
DBUA_M	dB μ A/m
AMPS	Amps

NOTE. Select dB μ V/m or dB μ A/m unit when using an antenna table.

Examples UNIT:POWer DBM specifies the fundamental unit of power as dBm.

*WAI (No Query Form)

Prevents the analyzer from executing further commands or queries until all pending operations finish. This command allows you to synchronize the

operation of the analyzer with your application program. For the details, refer to *Synchronizing Execution* (See page 3-12.).

Conditions Measurement views: All

Group IEEE common commands

Syntax *WAI

Related Commands *OPC

Arguments None

Status and Events

Status and Events

The SCPI interface in the analyzer includes a status and event reporting system that enables the user to monitor crucial events that occur in the instrument. The analyzer is equipped with four registers and one queue that conform to IEEE Std 488.2-1987. This section will discuss these registers and queues along with status and event processing.

Status and Event Reporting System

The following figure outlines the status and event reporting mechanism offered in the RSA6100A Series analyzers. It contains three major blocks

- Standard Event Status
- Operation Status
- Questionable Status (fan-out structure)

The processes performed in these blocks are summarized in the Status Byte. The three blocks contain four types of registers as shown in the following table.

Table 3-1: Register type

Register	Description
Condition register	Records event occurrence in the instrument. Read only.
Transition register (positive/negative)	A positive transition filter allows an event to be reported when a condition changes from false to true. A negative filter allows an event to be reported when a condition changes from true to false. Setting both positive and negative filters true allows an event to be reported anytime the condition changes. Clearing both filters disables event reporting.
Event register	Records events filtered by the transition register. Read only.
Enable register	Masks the event register to report in the summary bit. User-definable.

* The use of Bit 15 is not allowed in SCPI.
 The value of this bit is always zero.

CR: Condition Register
 TR: Transition Register
 EVR: Event Register
 ENR: Enable Register

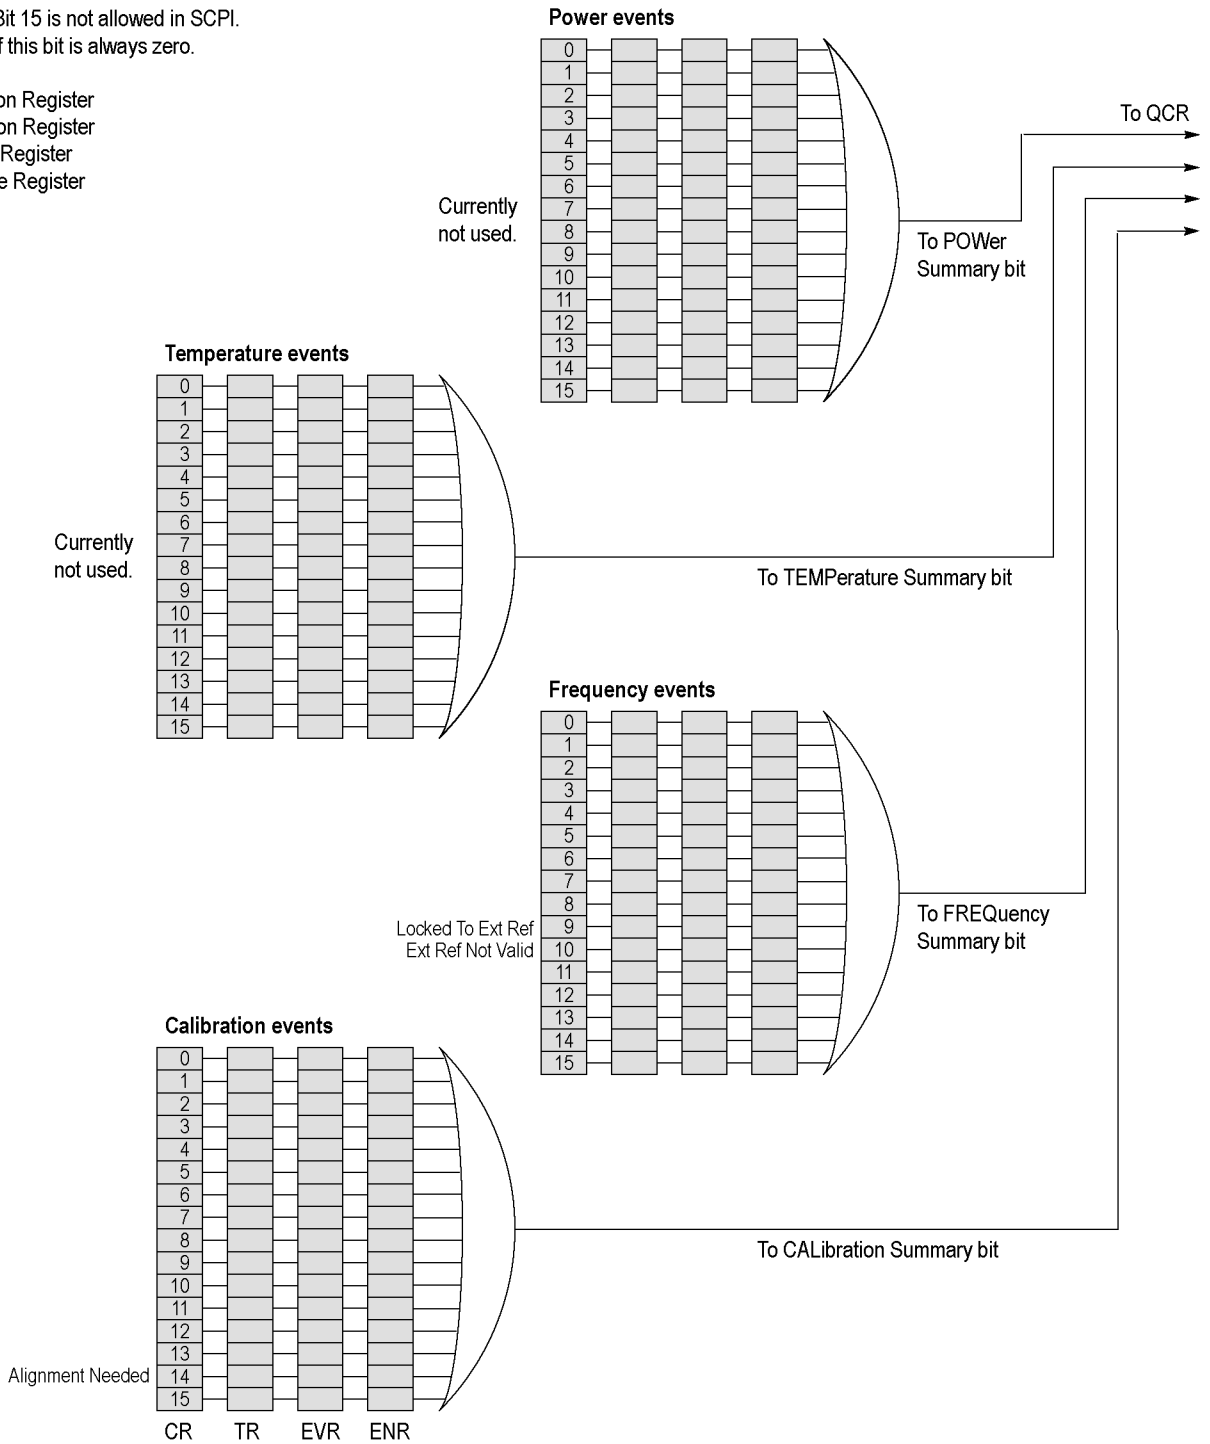


Figure 3-1: Status/Event reporting mechanism

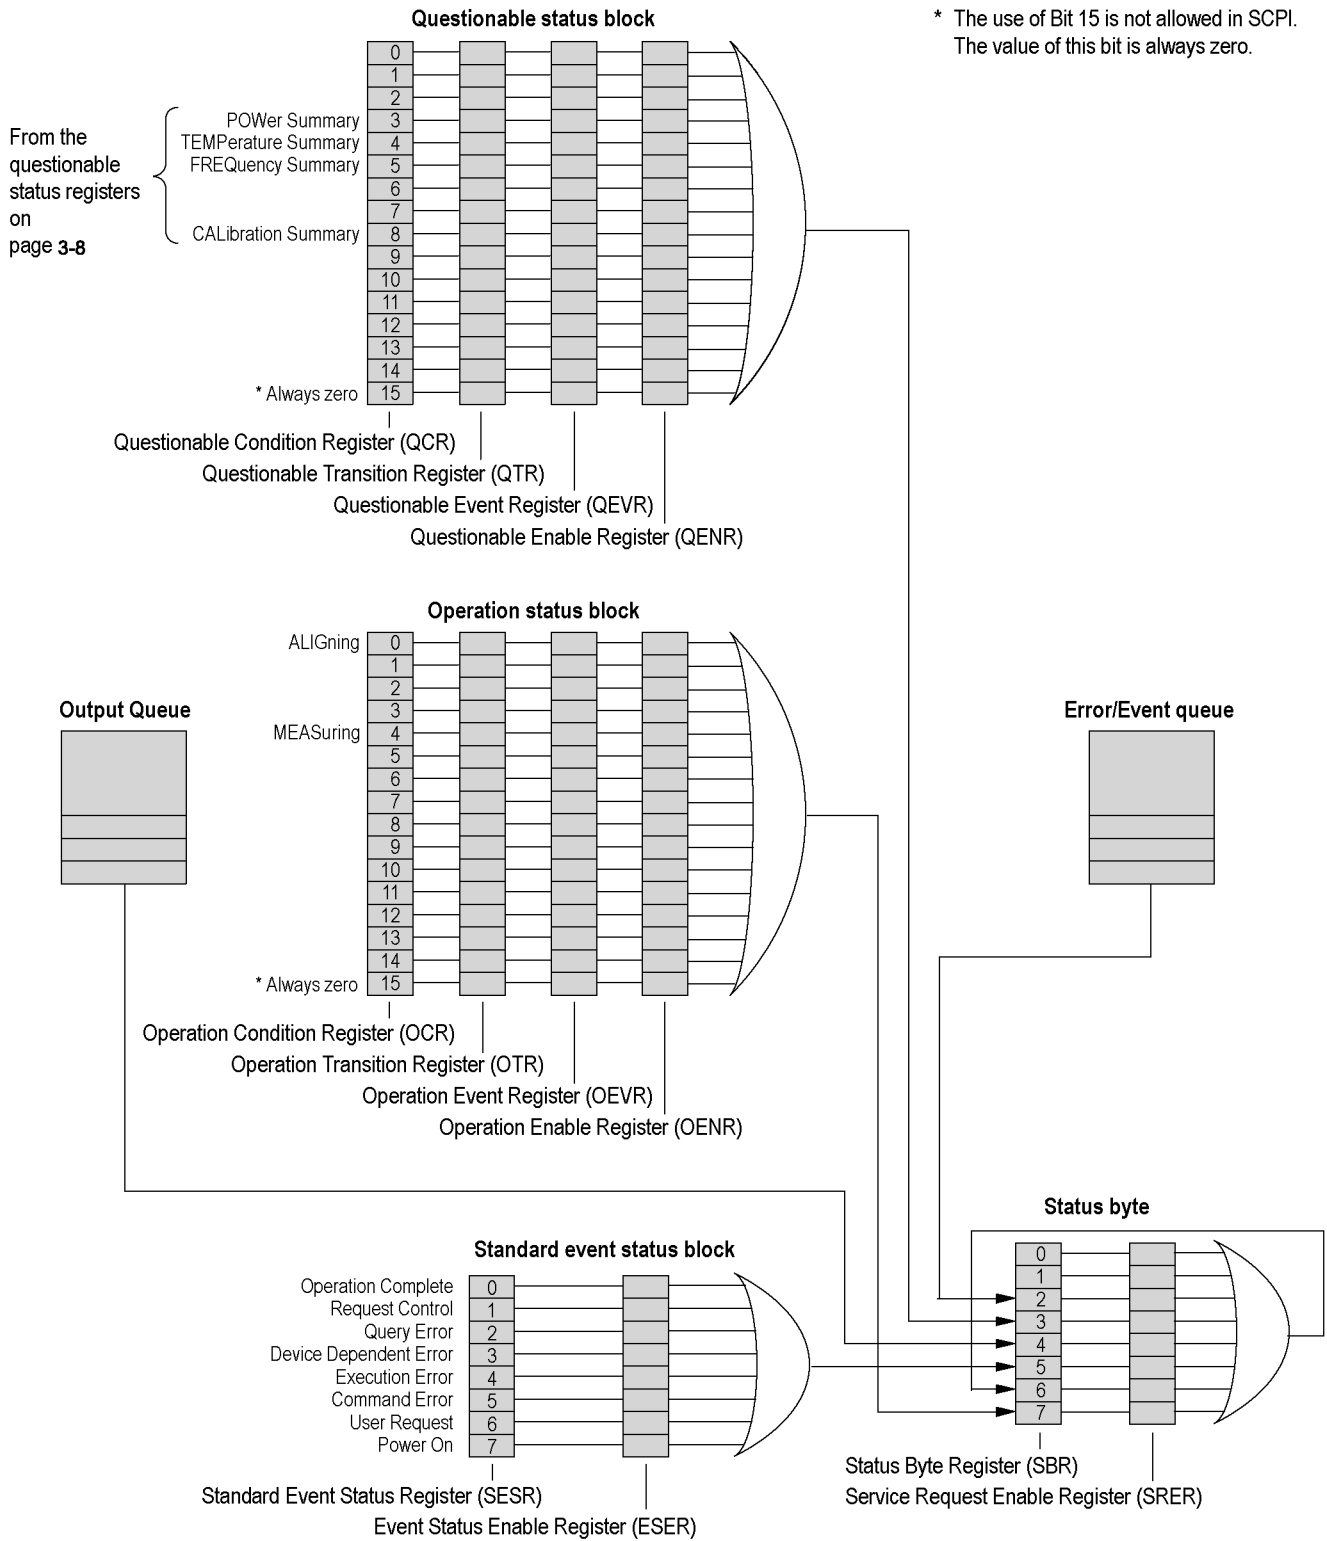


Figure 3-2: Status/Event reporting mechanism (Cont.)

Status Byte

The Status Byte contains the following two registers

- Status Byte Register (SBR)
- Service Request Enable Register (SRER)

Status Byte Register (SBR)

The SBR is made up of 8 bits. Bits 4, 5 and 6 are defined in accordance with IEEE Std 488.2-1987. These bits are used to monitor the output queue, SESR and service requests, respectively. The contents of this register are returned when the *STB? query is used.

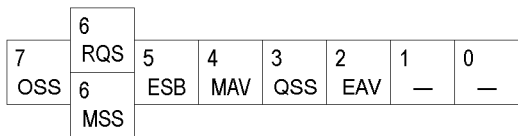


Figure 3-3: Status Byte Register (SBR)

Table 3-2: SBR bit functions

Bit	Description
7	Operation Summary Status (OSS). Summary of the operation status register.
6	Request Service (RQS)/Master Status Summary (MSS). When the instrument is accessed using the GPIB serial poll command, this bit is called the Request Service (RQS) bit and indicates to the controller that a service request has occurred (in other words, that the GPIB bus SRQ line is LOW). The RQS bit is cleared when serial poll ends. When the instrument is accessed using the *STB? query, this bit is called the Master Status Summary (MSS) bit and indicates that the instrument has issued a service request for one or more reasons. The MSS bit is never cleared to 0 by the *STB? query.
5	Event Status Bit (ESB). This bit indicates whether or not a new event has occurred after the previous Standard Event Status Register (SESR) has been cleared or after an event readout has been performed.
4	Message Available Bit (MAV). This bit indicates that a message has been placed in the output queue and can be retrieved.
3	Questionable Summary Status (QSS). Summary of the Questionable Status Byte register.
2	Event Quantity Available (EAV). Summary of the Error Event Queue.
1-0	Not used

Service Request Enable Register (SRER)

The SRER is made up of bits defined exactly the same as bits 0 through 7 in the SBR as shown in the following figure. This register is used by the user to determine what events will generate service requests.

The SRER bit 6 cannot be set. Also, the RQS is not maskable.

The generation of a service request with the GPIB interface involves changing the SRQ line to LOW and making a service request to the controller. The result is that a status byte for which an RQS has been set is returned in response to serial polling by the controller.

Use the *SRE command to set the bits of the SRER. Use the *SRE? query to read the contents of the SRER. Bit 6 must normally be set to 0.

7	6	5	4	3	2	1	0
OSB	—	ESB	MAV	QSB	—	—	—

Figure 3-4: Service Request Enable Register (SRER)

Standard Event Status Block

Reports the power on/off state, command errors, and the running state. It consists of the following registers

- Standard Event Status Register (SESR)
- Event Status Enable Register (ESER)

These registers are made up of the same bits defined in the following figure and table. Use the *ESR? query to read the contents of the SESR. Use the *ESE() command to access the ESER.

7	6	5	4	3	2	1	0
PON	—	CME	EXE	DDE	QYE	—	OPC

Figure 3-5: Standard event status register

Table 3-3: Standard event status register bit definition

Bit	Description
7	Power On (PON). Indicates that the power to the instrument is on.
6	Not used.
5	Command Error (CME). Indicates that a command error has occurred while parsing by the command parser was in progress.
4	Execution Error (EXE). Indicates that an error occurred during the execution of a command. Execution errors occur for one of the following reasons <ul style="list-style-type: none"> ■ When a value designated in the argument is outside the allowable range of the instrument, or is in conflict with the capabilities of the instrument. ■ When the command could not be executed properly because the conditions for execution differed from those essentially required.
3	Device-Dependent Error (DDE). An instrument error has been detected.
2	Query Error (QYE). Indicates that a query error has been detected by the output queue controller. Query errors occur for one of the following reasons <ul style="list-style-type: none"> ■ An attempt was made to retrieve messages from the output queue, despite the fact that the output queue is empty or in pending status. ■ The output queue messages have been cleared despite the fact that they have not been retrieved.
1	Not used.
0	Operation Complete (OPC). This bit is set with the results of the execution of the *OPC command. It indicates that all pending operations have been completed.

When an event occurs, the SESR bit corresponding to the event is set, resulting in the event being stacked in the Error/Event Queue. The SBR OAV bit is also set. If the bit corresponding to the event has also been set in the ESER, the SBR ESB bit is also set. When a message is sent to the Output Queue, the SBR MAV bit is set.

Operation Status Block

The operation status block contains conditions that are part of the instrument's normal operation. It consists of the following registers

- Operation Condition Register (OCR)
- Operation Positive/ Negative Transition Register (OPTR/ONTR)
- Operation Event Register (OEVR)
- Operation Enable Register (OENR)

These registers are made up of the same bits defined in the following table and figure. Use the STATUS:OPERation commands to access the operation status register set.

15	14	13	12	11	10	9	8	7	6	5	4	3	2	1	0
											MEAS				ALIG

Figure 3-6: Operation status register

Table 3-4: Operation status register bit definition

Bit	Description
15	Always zero (0).
14 - 5	Not used.
4	Measuring (MEAS). Indicates that the instrument is actively measuring. When the measurement ends after this bit is set in measurement, it is reset. "In measurement" means that one of the following commands is in execution: <ul style="list-style-type: none"> ■ INITiate commands ■ READ commands
3 - 1	Not used.
0	Aligning (ALIG). Indicates that the instrument is currently performing an alignment. When the alignment ends after this bit is set in alignment, it is reset.

When the specified state changes in the OCR, its bit is set or reset. This change is filtered with a transition register, and the corresponding bit of the OEVR is set. If the bit corresponding to the event has also been set in the OENR, the SBR OSS bit is also set.

Questionable Status Block

The questionable status register set contains bits which give an indication of the quality of various aspects of the signal together with the fanned out registers as described in the next subsections. It consists of the following registers

- Questionable Condition Register (QCR)
- Questionable Positive/Negative Transition Register (QPTR/QNTR)
- Questionable Event Register (QEVN)
- Questionable Enable Register (QENR)

These registers are made up of the same bits defined in the following table and figure. Use the STATUS:QUESTionable commands to access the questionable status register set.

15	14 CW	13	12	11	10	9	8 CAL	7	6	5 FREQ	4 TEMP	3 POW	2	1	0
----	----------	----	----	----	----	---	----------	---	---	-----------	-----------	----------	---	---	---

Figure 3-7: Questionable status register

Table 3-5: Questionable status register bit definition

Bit	Description
15	Always zero (0).
14	Command Warning (CW). Indicates a non-fatal warning that relates to the instrument's interpretation of a command, query, or one or more parameters of a specific command or query.
13 - 9	Not used.
8	CALibration Summary (CAL). Summary of the Questionable Calibration register.
7, 6	Not used.
5	FREQuency Summary (FREQ). Summary of the Questionable Frequency register.
4	TEMPerature Summary (TEMP). Summary of the Questionable Temperature register.
3	POWER Summary (POW). Summary of the Questionable Power register.
2 - 0	Not used.

When the specified state changes in the QCR, its bit is set or reset. This change is filtered with a transition register, and the corresponding bit of the QEVN is set. If the bit corresponding to the event has also been set in the QENR, the SBR QSS bit is also set.

Questionable Power Register Set

Refines the power error for the POWER bit in the QCR.

Currently not used.

Questionable Temperature Register Set Refines the temperature error for the TEMPerature bit in the QCR.
Currently not used.

Questionable Frequency Register Set The questionable frequency register set is made up of bits defined in the following table and figure. It refines the frequency error for the FREQuency bit in the QCR. Use the STATus:QUEStionable:FREQuency commands to access the questionable frequency register set.

15	14	13	12	11	10 ERNV	9 LTER	8	7	6	5	4	3	2	1	0
----	----	----	----	----	------------	-----------	---	---	---	---	---	---	---	---	---

Figure 3-8: Questionable frequency status register

Table 3-6: Questionable frequency status register bit definition

Bit	Description
15	Always zero (0).
14 - 11	Not used.
10	External Ref Not Valid (ERNV). Indicates that the external reference signal is not valid so the instrument is no longer locked to it.
9	Locked To External Ref (LTER). Indicates that the instrument is locked to the external reference signal.
8 - 0	Not used.

Questionable Calibration Register Set The questionable calibration register set is made up of bits defined in the following table and figure. It refines the calibration error for the CALibration bit in the QCR. Use the STATus:QUEStionable:CALibration commands to access the questionable calibration register set.

15	14 ALN	13	12	11	10	9	8	7	6	5	4	3	2	1	0
----	-----------	----	----	----	----	---	---	---	---	---	---	---	---	---	---

Figure 3-9: Questionable calibration status register

Table 3-7: Questionable calibration status register bit definition

Bit	Description
15	Always zero.
14	Alignment Needed (ALN). Indicates the instrument needs the alignment.
13 - 0	Not used.

Queues

There are two types of queues in the status reporting system used in the analyzer: output queues and event queues.

Output Queue

The output queue is a FIFO (first in, first out) queue and holds response messages to queries, where they await retrieval. When there are messages in the queue, the SBR MAV bit is set.

The output queue will be emptied each time a command or query is received, so the controller must read the output queue before the next command or query is issued. If this is not done, an error will occur and the output queue will be emptied; however, the operation will proceed even if an error occurs.

Event Queue

The event queue is a FIFO queue and stores events as they occur in the analyzer. If more than 32 events occur, event 32 will be replaced with event code -350 ("Queue Overflow"). The error code and text are retrieved using the SYSTem:ERRor queries.

Status and Event Processing Sequence

The following figure shows an outline of the sequence for status and event processing.

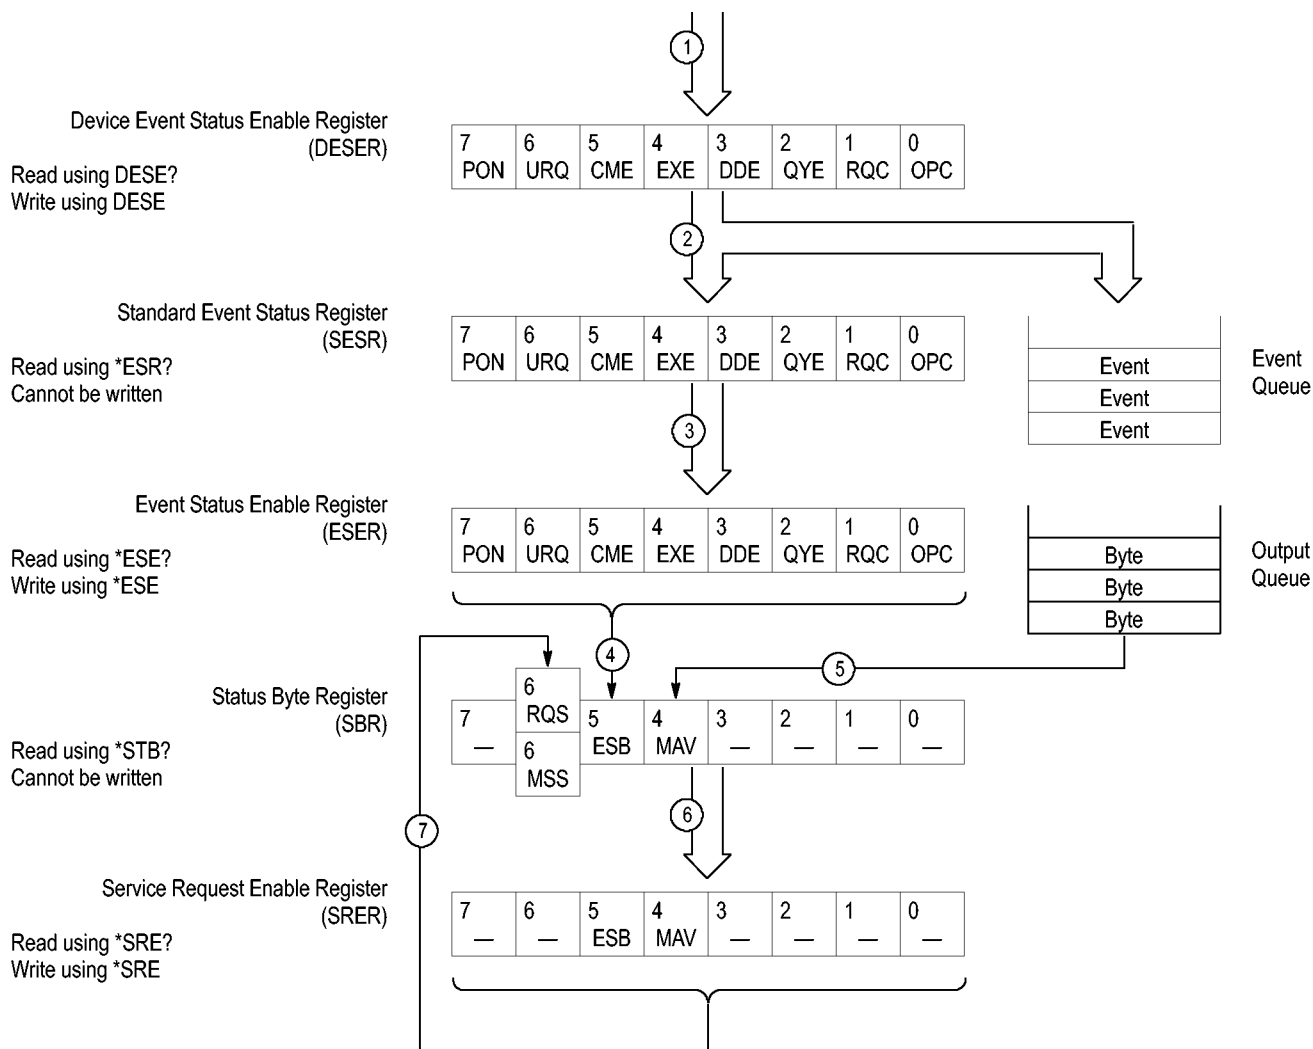


Figure 3-10: Status and event processing sequence

1. If an event has occurred, the SESR bit corresponding to that event is set and the event is placed in the event queue.
2. A bit corresponding to that event in the ESER has is set.
3. The SBR ESB bit is set to reflect the status of the ESER.
4. When a message is sent to the output queue, the SBR MAV bit is set.

5. Setting either the ESB or MAV bits in the SBR sets the respective bit in the SRER.
6. When the SRER bit is set, the SBR MSS bit is set and a service request is generated when using the GPIB interface.

Synchronizing Execution

Almost all commands are executed in the order in which they are sent from the controller, and the execution of each command is completed in a short period of time. However, the following commands perform data analysis in another thread, and another command can thus be executed concurrently

- INITiate commands
- READ commands
- [SENSe]:REANalyze

These commands are designed so that the next command to be sent is executed without waiting for the previous command to be completed. In some cases, a process executed by another command must first be completed before these commands can be executed; in other cases, these commands must be completed before the next command is executed.

You have two options to achieve command synchronization

- Using the status and event reporting function
- Using synchronizing commands

Using the Status and Event Reporting Function

In the following example, a READ command is used to obtain the measurement results while the Operation Condition Register (OCR) is being used to provide synchronization.

```

STATUS:OPERation:NTRansition 16
    // Set the filter of the OCR MEASuring bit
STATUS:OPERation:ENABle 16
    // Enable the filter of the OCR MEASuring bit
*SRE 128
    // Set the SRER OSS bit
READ:SPECTrum:TRACe
    // Obtain the measurement results
    
```

The command waits for generation of SRQ.

Using Synchronizing Commands

The IEEE-488.2 common commands include the following synchronizing commands

- *OPC
- *OPC?
- *WAI

Using the *OPC command. The *OPC command sets the SESR OPC bit when all the operations for which it is waiting are completed. If the GPIB interface is in use, you can synchronize the execution by using this command together with the serial polling or service request function.

The following is a command sequence example:

```
*ESE 1
  // Enable the ESER OPC bit
*SRE 32
  // Enable the SRER ESB bit
ABORt;INITiate:IMMediate;*OPC
  // Wait for SRQ to provide synchronization
```

Using the *OPC? query. The query *OPC? writes ASCII code "1" into the Output Queue when all operations for which it is waiting are completed. You can provide synchronization using the command string as the following example:

```
ABORt;INITiate:IMMediate;*OPC
```

The command waits until "1" is written into the Output Queue. When the command goes to the Output Queue to read the data, a time-out may occur before the data is written into the queue.

Using the *WAI Command. After the process of the preceding command is completed, the *WAI command begins to execute the process of the next command as the following example:

```
ABORt;INITiate:IMMediate;*WAI
  // Wait for the *WAI process to provide synchronization
```

Error Messages and Codes

Error codes with a negative value are SCPI standard error codes; errors with a positive value are unique to the RSA6100A Series Real-Time Spectrum Analyzers.

Event codes and messages can be obtained by using the queries `SYSTEM:ERROR?` and `SYSTEM:ERROR:ALL?` These are returned in the following format

```
<event_code>,"<event_message>"
```

Command Errors

Command errors are returned when there is a syntax error in the command.

Table 3-8: Command errors

Error code	Error message
-100	Command error
-101	Invalid character
-102	Syntax error
-103	Invalid separator
-104	Data type error
-105	GET not allowed
107	Can't replay - settings not compatible with data record
-109	Missing parameter
-111	Header separator error
-112	Program mnemonic too long
-113	Undefined header
-114	Header suffix out of range
-120	Numeric data error
-121	Character
-123	Exponent too large
-124	Too many digits
-128	Numeric data not allowed
-130	Suffix error
-131	Invalid suffix
-134	Suffix too long
-138	Suffix not allowed
-140	Character data error
-141	Invalid character data
-144	Character data too long
-148	Character data not allowed

Table 3-8: Command errors (cont.)

Error code	Error message
-150	String data error
-151	Invalid string data
-158	String data not allowed
-160	Block data error
-161	Invalid block data
-168	Block data not allowed
-170	Command expression error
-171	Invalid expression
-178	Expression data not allowed
-180	Macro error
-181	Invalid outside macro definition
-183	Invalid inside macro definition
-184	Macro parameter error

Execution Errors

These error codes are returned when an error is detected while a command is being executed.

Table 3-9: Execution errors

Error code	Error message
-200	Execution error
-201	Invalid while in local
-202	Settings lost due to RTL
-210	Trigger error
-211	Trigger ignored
-212	Arm ignored
-213	Init ignored
-214	Trigger deadlock
-215	Arm deadlock
-220	Parameter error
-221	Settings conflict
-222	Data out of range
-223	Too much data
-224	Illegal parameter value
-225	Out of memory
-226	Lists not same length

Table 3-9: Execution errors (cont.)

Error code	Error message
-230	Data corrupt or stale
-231	Data questionable
-240	Hardware error
-241	Hardware missing
-250	Mass storage error
-251	Missing mass storage
-252	Missing media
-253	Corrupt media
-254	Media full
-255	Directory full
-256	Filename not found
-257	Filename error
-258	Media protected
-260	Execution expression error
-261	Math error in expression
-270	Execution macro error
-271	Macro syntax error
-272	Macro execution error
-273	Illegal macro label
-274	Execution macro parameter error
-275	Macro definition too long
-276	Macro recursion error
-277	Macro redefinition not allowed
-278	Macro header not found
-280	Program error
-281	Cannot create program
-282	Illegal program name
-283	Illegal variable name
-284	Program currently running
-285	Program syntax error
-286	Program runtime error

Device Specific Errors

These error codes are returned when an internal instrument error is detected. This type of error may indicate a hardware problem.

Table 3-10: Device specific errors

Error code	Error message
-300	Device specific error
-310	System error
-311	Memory error
-312	PUD memory lost
-313	Calibration memory lost
-314	Save/Recall memory lost
-315	Configuration memory lost
-330	Self test failed
-350	Queue overflow

Query Errors

These error codes are returned in response to an unanswered query.

Table 3-11: Query errors

Error code	Error message
-400	Query error
-410	Query interrupted
-420	Query untermiated
-430	Query deadlocked
-440	Query untermiated after indefinite period

Device Errors

These error codes are unique to the RSA6100A Series. They are classified into three groups: global, measurement, and source conditions, as shown in the following tables.

Table 3-12: Device errors, global condition

Error code	Error message
100	Setup error
101	Disabled: data is from swept acquisition
102	Disabled: swept settings; Acquire data while display is selected
103	Acquisition bandwidth too small for current setup
104	Can't get acquisition data record
105	Can't open the requested display
106	Analysis failure
107	Analysis length was limited
108	Analysis length too small for current setup
109	No math trace: unmatched trace lengths
110	Analysis time was adjusted
111	Not enough samples for current setup
112	Can't replay. Data is from swept acquisition.
113	Can't replay. Live data needed for swept settings.
114	Recall error: setup not completely restored
115	Recall failure: problem with file or file contents
116	Save failure: file not saved
117	Unexpected software error. Please cycle power and try again.
118	Export failure: file not saved
119	Export failure: unable to open results file for export. File not saved.
120	Search condition for this result is already defined.
121	Search condition for this result was not found.
124	Load failed: <filename>
125	Store error: file not saved.
126	No Math trace: unmatched trace X range
127	Not enough memory for measurement
128	Incomplete analysis
129	Not enough samples for current setup
130	Mask creation error: <reason message>

Table 3-13: Device errors, measurement condition

Error code	Error message
1000	TDBW actual (TDBW: Time Domain Bandwidth)
1002	RBW increased to
1003	RBW limited by acquisition bandwidth to
1004	RBW conflict. Increase span or analysis length
1011	Audio disabled: configuration problem
1012	Audio Demod disabled: swept acquisition
1013	Audio Demod disabled: trigger in use
1014	Audio disabled: IF band outside Acq BW
1015	Calibration error. See Windows Event Viewer for error detail.
OBW errors	
1016	Analysis failure: $\text{AcqBW} < \text{MeasBW} + (5 \times \text{RBW})$
1017	Analysis failure: AcqBW must be 10 kHz or more
1018	$x \text{ dB BW} > \text{Meas BW}$
Pulse errors	
1019	AcqBW too low for current Chirp BW setting
1020	Impulse Response only valid for Chirp modulation
1023	Not enough memory for measurement
Other measurements	
1024	BW actual (limited by Acq BW)
1025	CISPR not available in FastFrame. Uncheck FastFrame in the Acquire panel.
1026	Analysis length must be in auto.
1027	Carrier not found
1029	CISPR accuracy limited by acq memory. Adjust RBW or freq range.
1030	CISPR: Acq BW too small for RBW. Try increasing span or freq range.
1031	Insufficient data for CISPR. Acquire while display is selected.
1032	VBW increased - Analysis Length too short
1033	VBW does not use full Analysis Length.
1034	Analysis time was adjusted Reached sample limit of

Table 3-14: Device errors, source condition

Error code	Error message
2008	Not calibrated
2009	FMT RBW limited by Acq BW to <XX>
2010	FMT RBW increased by Acq BW to <XX>
2011	Hardware failure - see Windows Event Viewer
2012	FMT disabled: Acq BW too small for current setup
2013	Hardware failure detected by diagnostics
2014	FMT disabled: RefLev too low for Volts/Watts units
2015	FMT disabled: settings conflict with selected measurement
2016	Preamp freq range exceeded
2024	RBW limited by Span to <XX>
2025	RBW increased by Span to <XX>
2028	External frequency reference signal not valid. Using internal reference.
2029	Unable to lock to external frequency reference. Using internal reference.
2033	Alignment error. Please run alignment again. If the problem persists, contact your Tektronix Service Center.
2034	Operational error: unable to complete operation. Please try again. If the problem persists, contact your Tektronix Service Center. See Windows Event Viewer for error detail.
2035	Hardware error: unable to configure hardware. Please try again. If the problem persists, contact your Tektronix Service Center. See Windows Event Viewer for error detail.
2036	Shutting down - internal temperature is too high. Check fans and airflow. If the problem persists, contact your Tektronix Service Center.
2037	Hardware error detected. To clear error, exit and restart the application. If the problem persists, contact your Tektronix Service Center.
2038	Disabled: RefLev too low\nfor Volts/Watts units
2042	Ext Corr > 20 dB pk-pk in acq segment
2044	Combined External Correction tables exceed the 60 dB peak-to-peak limit. External Correction tables were disabled. Please check table values and try again.
2045	Disabled: FastFrame doesn't support swept settings.
2046	Attenuator use currently exceeds the cautionary limit of 1200 changes per hour. Operation was stopped to protect against premature wear-out. The monitor function can be temporarily disabled in the Amplitude control panel or over the programmatic interface. Specified lifetime for an attenuator is 10,000,000 changes.
2047	Disabled: settings conflict with selected measurement

Status Conditions

Status conditions do not appear in the event queue, they are only returned by a :STATUS:<measurement>EVENTs? query.

Global Status

Global status conditions can be returned with any :STATUS:<measurement>EVENTs? query.

Table 3-15: Global status conditions

Status code	Status message
10107	Analysis Length was limited
10108	Analysis length too small for current setup
10110	Analysis time was adjusted
10122	Search result not enabled
10123	Search result no longer available

Measurement Status

Measurement status conditions are unique to specific measurement groups.

Table 3-16: Measurement status conditions

Status code	Status message
Pulse Measurements	
11001	Avg Tx only available in power units
11005	Pulse detection error
11006	Setup error: Define > Measurement Point is too late
11007	No pulses found
11008	No FFT (not all pulses have results)
11020	No FFT (not enough pulses)
11022	Analysis time was adjusted - reached time limit
11039	No sidelobe found
GP Digital Modulation	
11009	No burst detected
11034	Display not valid for selected modulation type
11035	Samples per symbol > 200. Decrease Measurement BW
11036	Too many samples per symbol. Decrease Measurement BW

Table 3-16: Measurement status conditions (cont.)

Status code	Status message
Chan Power and ACPR	
11010	Measuring Noise
Other	
11028	CISPR: (progress message)
11037	Ext corrections enabled for traces

Source Status

Source status conditions can be returned with any :STATus:<measurement>EVENTs? query.

Table 3-17: Source status conditions

Status code	Status message
12000	Data acquired during RF ADC overrange
12005	Aligning
12006	Not aligned
12007	Unaligned data
12009	Data from uncalibrated instrument
12010	Dither: manual control
12012	Data acquired during hardware failure
12014	Data acquired during RF dig gain overflow
12015	Locking to ext freq ref signal...
12018	RF Attenuator: manual control
12019	Saving acquisition
12020	Recalling acquisition data
12022	Disabled: data is from swept acquisition
12023	Disabled: Freq Mask Trigger in use
12026	Acq Sampling params: manual control
12027	Swept: RF Trig invalid for most signals
12030	Data acquired during RF ADC overrange
12031	Data acquired during RF dig gain overflow
12039	Decrease RefLev or increase\nAtten to prevent data errors
12040	Possible data errors - acquired with RefLev too much higher than RFAtten
12043	Ext Corr error - tables not applied
12056	Warming up
12057	Data acquired during warm-up
12063	Triggers disabled when DPX is swept


Table 3-17: Source status conditions (cont.)

Status code	Status message
12064	Waiting for trigger. Open the DPX display.
12066	Data exceeds preamp range

Appendices

Appendix A: Character Charts

B7 B6 B5 BITS B4 B3 B2 B1	0 0		0 0 1		0 1 0		0 1 1		1 0 0		1 0 1		1 1 0		1 1 1	
	CONTROL				NUMBERS SYMBOLS				UPPER CASE				LOWER CASE			
0 0 0 0	0 NUL	20 DLE	40 SP	60 0	100 @	120 P	140 ' SA0	160 p SA16	0	0	0	0	0	0	0	0
0 0 0 1	1 SOH	21 DC1	41 !	61 1	101 A	121 Q	141 a SA1	161 q SA17	1	1	1	1	1	1	1	1
0 0 1 0	2 STX	22 DC2	42 "	62 2	102 B	122 R	142 b SA2	162 r SA18	2	2	2	2	2	2	2	2
0 0 1 1	3 ETX	23 DC3	43 #	63 3	103 C	123 S	143 c SA3	163 s SA19	3	3	3	3	3	3	3	3
0 1 0 0	4 EOT	24 DC4	44 \$	64 4	104 D	124 T	144 d SA4	164 t SA20	4	4	4	4	4	4	4	4
0 1 0 1	5 ENQ	25 NAK	45 %	65 5	105 E	125 U	145 e SA5	165 u SA21	5	5	5	5	5	5	5	5
0 1 1 0	6 ACK	26 SYN	46 &	66 6	106 F	126 V	146 f SA6	166 v SA22	6	6	6	6	6	6	6	6
0 1 1 1	7 BEL	27 ETB	47 ' LA7	67 7	107 G	127 W	147 g SA7	167 w SA23	7	7	7	7	7	7	7	7
1 0 0 0	8 BS	30 CAN	50 (LA8	70 8	110 H	130 X	150 h SA8	170 x SA24	8	8	8	8	8	8	8	8
1 0 0 1	9 HT	31 EM	51) LA9	71 9	111 I	131 Y	151 i SA9	171 y SA25	9	9	9	9	9	9	9	9
1 0 1 0	A LF	32 SUB	52 * LA10	72 :	112 J	132 Z	152 j SA10	172 z SA26	A	A	A	A	A	A	A	A
1 0 1 1	B VT	33 ESC	53 + LA11	73 ; LA27	113 K	133 [153 k SA11	173 { SA27	B	B	B	B	B	B	B	B
1 1 0 0	C FF	34 FS	54 , LA12	74 < LA28	114 L	134 \	154 l SA12	174 SA28	C	C	C	C	C	C	C	C
1 1 0 1	D CR	35 GS	55 - LA13	75 = LA29	115 M	135]	155 m SA13	175 } SA29	D	D	D	D	D	D	D	D
1 1 1 0	E SO	36 RS	56 . LA14	76 > LA30	116 N	136 ^	156 n SA14	176 ~ SA30	E	E	E	E	E	E	E	E
1 1 1 1	F SI	37 US	57 / LA15	77 ? UNL	117 O	137 -	157 o SA15	177 RUBOUT (DEL)	F	F	F	F	F	F	F	F
	ADDRESSED COMMANDS	UNIVERSAL COMMANDS	LISTEN ADDRESSES	TALK ADDRESSES	SECONDARY ADDRESSES OR COMMANDS											



Tektronix
 REF: ANSI STD X3.4-1977
 IEEE STD 488.1-1987
 ISO STD 646-2973

Appendix B: GPIB Interface Specification

This appendix lists and describes the GPIB functions and messages the instrument can implement.

Interface Functions

The following table lists the GPIB interface functions this instrument implements. Each function is briefly described.

Table B-1: GPIB interface function implementation

Interface function	Implemented subset	Capability
Source Handshake (SH)	SH1	Complete
Acceptor Handshake (AH)	AH1	Complete
Talker (T)	T6	Basic Talker, Serial Poll Unaddress if my-listen-address (MLA) No Talk Only mode
Listener (L)	L4	Basic Listener Unaddress if my talk address (MTA) No Listen Only mode
Service Request (SR)	SR1	Complete
Remote/Local (RL)	RL0	None
Parallel Poll (PP)	PP0	None
Device Clear (DC)	DC1	Complete
Device Trigger (DT)	DT0	None
Controller (C)	C0	None
Electrical Interface	E2	Three-state driver

- Source Handshake (SH). Enables a talking device to support the coordination of data transfer. The SH function controls the initiation and termination of data byte transfers.
- Acceptor Handshake (AH). Enables a listening device to coordinate data reception. The AH function delays data transfer initiation or termination until the listening device is ready to receive the next data byte.
- Talker (T). Enables a device to send device-dependent data over the interface. This capability is available only when the device is addressed to talk, and uses a one-byte address.
- Listener (L). Enables a device to receive device-dependent data over the interface. This capability is available only when the device is addressed to listen, and uses a one-byte address.
- Service Request (SR). Enables a device to assert an SRQ (Service Request) line to notify the controller when it requires service.
- Remote/Local (RL). Enables a device to respond to both the GTL (Go To Local) and LLO (Local Lock Out) interface messages.
- Parallel Poll (PP). Enables a device to respond to the following interface messages: PPC, PPD, PPE, and PPU, as well as to send out a status message when the ATN (Attention) and EOI (End or Identify) lines are asserted simultaneously.
- Device Clear (DC). Enables a device to be cleared or initialized, either individually, or as part of a group of devices.
- Device Trigger (DT). Enables a device to respond to the GET (Group Execute Trigger) interface message when acting as a listener.
- Controller (C). Enables a device that has this capability to send its address, universal commands, and addressed commands to other devices over the interface.
- Electrical Interface (E). Identifies the electrical interface driver type. The notation E1 means the electrical interface uses open collector drivers, E2 means the electrical interface uses three-state drivers.

Interface Messages

Table B-2: Standard interface messages

Message	Type ¹	Implemented
Device Clear (DCL)	UC	Yes
Local Lockout (LLO)	UC	No
Serial Poll Disable (SPD)	UC	Yes
Serial Poll Enable (SPE)	UC	Yes
Parallel Poll Unconfigure (PPU)	UC	No
Go To Local (GTL)	AC	Yes
Selected Device Clear (SDC)	AC	Yes
Group Execute Trigger (GET)	AC	No
Take Control (TCT)	AC	No
Parallel Poll Configure (PPC)	AC	No

¹ UC: Universal command; AC: Address command

- Device Clear (DCL). Will clear (initialize) all devices on the bus that have a device clear function, whether or not the controller has addressed them.
- Local Lockout (LLO). Disables the return to local function.
- Serial Poll Disable (SPD). Changes all devices on the bus from the serial poll state to the normal operating state.
- Serial Poll Enable (SPE). Puts all bus devices that have a service request function into the serial poll enabled state. In this state, each device sends the controller its status byte, instead of its normal output, after the device receives its talk address on the data lines. This function may be used to determine which device sent a service request.
- Go To Local (GTL). Causes the listen-addressed device to switch from remote to local (front-panel) control.
- Select Device Clear (SDC). Clears or initializes all listen-addressed devices.
- Group Execute Trigger (GET). Triggers all applicable devices and causes them to initiate their programmed actions.
- Take Control (TCT). Allows the controller in charge to pass control of the bus to another controller on the bus.
- Parallel Poll Configure (PPC). Causes the listen-addressed device to respond to the secondary commands Parallel Poll Enable (PPE) and Parallel Poll Disable (PPD), which are placed on the bus following the PPC command. PPE enables a device with parallel poll capability to respond on a particular data line. PPD disables the device from responding to the parallel poll.

Appendix C: Factory Initialization Settings

The factory initialization settings provide a known state for the analyzer. The *RST command returns the instrument settings to the factory defaults. Factory initialization sets values as shown in the following tables in this section.

Table C-1: Factory initialization settings, IEEE common commands

Header	Default value
*ESE	0
*OPC	0
*SRE	0

Table C-2: Factory initialization settings, Calculate commands

Header	Default value
CALCulate basic command subgroup	
CALCulate:MARKer:DENSity:EXCursion	50
CALCulate:MARKer:DENSity:SMOothing	5
CALCulate:MARKer:DENSity:THReshold	500
CALCulate:MARKer:MODE	ABSolute
CALCulate:MARKer:PEAK:EXCursion	6 dB
CALCulate:MARKer:PEAK:THReshold	-150 dBm
CALCulate:SEARch:LIMit:MATCH:BEEP[:STATe]	OFF
CALCulate:SEARch:LIMit:MATCH:SACQuire[:STATe]	OFF
CALCulate:SEARch:LIMit:MATCH:SDATa[:STATe]	OFF
CALCulate:SEARch:LIMit:MATCH:SPICture[:STATe]	OFF
CALCulate:SEARch:LIMit:MATCH:STRace[:STATe]	OFF
CALCulate:SEARch:LIMit:OPERation	GT
CALCulate:SEARch:LIMit:OPERation:FEED	"Spectrum", "Trace 1"
CALCulate:SEARch:LIMit:OPERation:SLIMit	-20 dBm
CALCulate:SEARch:LIMit:STATe	OFF
CALCulate:DPSA subgroup	
CALCulate:DPSA:MARKer<x>:TRACe	TRACE1
CALCulate:DPSA:MARKer<x>:X:AMPLitude	0 dBm
CALCulate:DPSA:MARKer<x>:X[:FREQuency]	1.5 GHz
CALCulate:SPECTrum subgroup	
CALCulate:SPECTrum:MARKer<x>:TRACe	TRACE1

Table C-3: Factory initialization settings, Calibration commands

Header	Default value
CALibration:AUTO	ON
CALibration:CORRection:EXTErnal:EDIT<x>:LABel	Ext Gain Table n
CALibration:CORRection:EXTErnal:EDIT<x>:STATe	OFF
CALibration:CORRection:EXTErnal:GAIN[:MAGNitude]	30 dB
CALibration:CORRection:EXTErnal:GAIN:STATe	OFF
CALibration:CORRection:EXTErnal:PROBe:STATe	OFF
INPut:CORRection:EXTErnal:EDIT<x>:INTErpolation	TRACe

Table C-4: Factory initialization settings, Display commands

Header	Default value
DISPlay basic command subgroup	
DISPlay:WINDow:COLor:SCHEme	CLASsic
DISPlay:ACPower subgroup	
DISPlay:ACPower:MARKer:SHOW:STATe	ON
DISPlay:ACPower:PLEVel:SHOW:STATe	ON
DISPlay:ACPower:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:ACPower:X[:SCALe]	13.84 MHz
DISPlay:ACPower:X[:SCALe]:OFFSet	1.5 GHz
DISPlay:ACPower:Y[:SCALe]	100 dB
DISPlay:ACPower:Y[:SCALe]:OFFSet	0
DISPlay:{AM FM PM} subgroup	
DISPlay:{AM FM PM}:MARKer:SHOW:STATe	ON
DISPlay:{AM FM PM}:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:AVTime subgroup	
DISPlay:AVTime:MARKer:SHOW:STATe	ON
DISPlay:AVTime:TRIGger:LEVel:STATe	ON
DISPlay:AVTime:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:AVTime:X[:SCALe]:AUTO:STATe	ON
DISPlay:AVTime:X[:SCALe]:OFFSet	0
DISPlay:AVTime:Y[:SCALe]:FULL	100 dB
DISPlay:AVTime:Y[:SCALe]:OFFSet	0
DISPlay:CONSte subgroup	
DISPlay:CONSte:MPHase	P1
DISPlay:CONSte:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:DDEMod subgroup	

Table C-4: Factory initialization settings, Display commands (cont.)

Header	Default value
DISPlay:DDEMod:RADix	BINary
DISPlay:DDEMod:X[:SCALe]	128 symbols
DISPlay:DDEMod:X[:SCALe]:AUTO:STATe	ON
DISPlay:DDEMod:X[:SCALe]:OFFSet	-1 symbol
DISPlay:DIQVtime subgroup	
DISPlay:DIQVtime:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:DPSA subgroup	
DISPlay:CCDF:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:DPSA:Y[:SCALe]:PDIVision	10 dB/div
DISPlay:EDiagram subgroup	
DISPlay:EDiagram:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:EVM subgroup	
DISPlay:EVM:Y[:SCALe]	100%
DISPlay:EVM:Y[:SCALe]:OFFSet	-100
DISPlay:FDVTime subgroup	
DISPlay:FDVTime:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:FVTime subgroup	
DISPlay:FVTime:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:FVTime:X[:SCALe]:AUTO:STATe	ON
DISPlay:FVTime:X[:SCALe]:OFFSet	0
DISPlay:FVTime:Y[:SCALe]	120 MHz
DISPlay:FVTime:Y[:SCALe]:OFFSet	0
DISPlay:GENeral subgroup	
DISPlay:GENeral:MEASview:SElect	SPECTrum
DISPlay:IQVTime subgroup	
DISPlay:IQVTime:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:IQVTime:X[:SCALe]:AUTO:STATe	ON
DISPlay:IQVTime:X[:SCALe]:OFFSet	0
DISPlay:IQVTime:Y[:SCALe]	10 V
DISPlay:IQVTime:Y[:SCALe]:OFFSet	0
DISPlay:MCPower subgroup	
DISPlay:MCPower:MARKer:SHOW:STATe	ON
DISPlay:MCPower:PLEVel:SHOW:STATe	ON
DISPlay:MCPower:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:MCPower:X[:SCALe]	38.84 MHz
DISPlay:MCPower:X[:SCALe]:OFFSet	1.5 GHz
DISPlay:MCPower:Y[:SCALe]	100 dB

Table C-4: Factory initialization settings, Display commands (cont.)

Header	Default value
DISPlay:MCPower:Y[:SCALe]:OFFSet	0
DISPlay:MERRor subgroup	
DISPlay:MERRor:Y[:SCALe]	100%
DISPlay:MERRor:Y[:SCALe]:OFFSet	-100
DISPlay:OBWidth subgroup	
DISPlay:OBWidth:MARKer:SHOW:STATe	ON
DISPlay:OBWidth:SELEcted:BANDwidth	OBWidth
DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe	ON
DISPlay:OBWidth:X[:SCALe]:OFFSet	0
DISPlay:OBWidth:Y[:SCALe]	100 dB
DISPlay:OBWidth:Y[:SCALe]:OFFSet	0
DISPlay:PERRor subgroup	
DISPlay:PERRor:Y[:SCALe]	360 (degrees)
DISPlay:PERRor:Y[:SCALe]:OFFSet	-360
DISPlay:PHVTime subgroup	
DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe	ON
DISPlay:PHVTime:X[:SCALe]:AUTO:STATe	ON
DISPlay:PHVTime:X[:SCALe]:OFFSet	0
DISPlay:PHVTime:Y[:SCALe]	1°
DISPlay:PHVTime:Y[:SCALe]:AXIS	MODulopi
DISPlay:PHVTime:Y[:SCALe]:AXIS:REFerence	0
DISPlay:PHVTime:Y[:SCALe]:OFFSet	0
DISPlay:PNOise subgroup	
DISPlay:PNOise:MARKer:SHOW:STATe	ON
DISPlay:PNOise:WINDow:TRACe:GRATicule:GRID:STATe	ON
DISPlay:PNOise:X[:SCALe]:START	10 Hz
DISPlay:PNOise:X[:SCALe]:STOP	1 GHz
DISPlay:PNOise:Y[:SCALe]	100 dB
DISPlay:PNOise:Y[:SCALe]:OFFSet	-50 dBc/Hz
DISPlay:PNOise:Y[:SCALe]:PDIVision	10 dB
DISPlay:PULSe subgroup	
DISPlay:PULSe:RESult:ATX	OFF
DISPlay:PULSe:RESult:AVERAge	ON
DISPlay:PULSe:RESult:DRODb	OFF
DISPlay:PULSe:RESult:DROOp	OFF
DISPlay:PULSe:RESult:DUTPct	OFF
DISPlay:PULSe:RESult:DUTRatio	OFF

Table C-4: Factory initialization settings, Display commands (cont.)

Header	Default value
DISPlay:PULSe:RESult:FALL	OFF
DISPlay:PULSe:RESult:FRDeviation	OFF
DISPlay:PULSe:RESult:IRAMplitude	OFF
DISPlay:PULSe:RESult:IRTime	OFF
DISPlay:PULSe:RESult:MFRqerror	OFF
DISPlay:PULSe:RESult:MPHerror	OFF
DISPlay:PULSe:RESult:OVEDb	OFF
DISPlay:PULSe:RESult:OVERshoot	OFF
DISPlay:PULSe:RESult:PHDeviation	OFF
DISPlay:PULSe:RESult:PPFRequency	OFF
DISPlay:PULSe:RESult:PPOWer	OFF
DISPlay:PULSe:RESult:PPPHas	OFF
DISPlay:PULSe:RESult:RINterval	OFF
DISPlay:PULSe:RESult:RIPDb	OFF
DISPlay:PULSe:RESult:RIPPl	OFF
DISPlay:PULSe:RESult:RISE	OFF
DISPlay:PULSe:RESult:RMSFReqerror	OFF
DISPlay:PULSe:RESult:RMSPherror	OFF
DISPlay:PULSe:RESult:RRATe	OFF
DISPlay:PULSe:RESult:TIME	OFF
DISPlay:PULSe:RESult:WIDTh	OFF
DISPlay:PULSe:SElect:NUMBer	0
DISPlay:PULSe:SElect:RESult	AVERAge
DISPlay:PULSe:STATistics:MARKer:SHOW:STATe	ON
DISPlay:PULSe:STATistics:PLOT	TRENd
DISPlay:PULSe:STATistics:WINDow:TRACe:GRATicule:GRID:STATe	ON
DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer	1
DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet	0
DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet	0
DISPlay:PULSe:STATistics:Y[:SCALE]:FULL	100 dB
DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet	0
DISPlay:PULSe:TRACe:MARKer:SHOW:STATe	ON
DISPlay:PULSe:TRACe:POINt:SHOW	ON
DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe	ON
DISPlay:PULSe:TRACe:X[:SCALE]:FULL	SElected
DISPlay:PULSe:TRACe:X[:SCALE]:OFFSet	0
DISPlay:PULSe:TRACe:X[:SCALE]:PDIVision	10 μ s

Table C-4: Factory initialization settings, Display commands (cont.)

Header	Default value
DISPlay:PULSe:TRACe:Y[:SCALe]:FULL	100 dB
DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet	0
DISPlay:SGRam subgroup	
DISPlay:SGRam:TIME:OFFSet	0
DISPlay:SGRam:TIME:OVERlap	ON
DISPlay:SGRam:TIME:SCALe	0
DISPlay:SPECtrum subgroup	
DISPlay:SPECtrum:FREQUency:OFFSet	1.5 GHz
DISPlay:SPECtrum:FREQUency[:SCALe]	40 MHz
DISPlay:SPECtrum:MARKer:NOISe:MODE	OFF
DISPlay:SPECtrum:SCALe:LOG:STATe	OFF
DISPlay:SPECtrum:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:PNOise:LEGend:STATe	OFF
DISPlay:SPECtrum:X:LABel	CFSPan
DISPlay:SPECtrum:Y[:SCALe]:PDIVision	10 dB/div
DISPlay:SPURious subgroup	
DISPlay:SPURious:MARKer:SHOW:STATe	ON
DISPlay:SPURious:SCALe:LOG:STATe	OFF
DISPlay:SPURious:SElect:NUMBer	1
DISPlay:SPURious:SHOW:LIMit	SHADed
DISPlay:SPURious:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:SPURious:X[:SCALe]:START	1.61 GHz
DISPlay:SPURious:X[:SCALe]:STOP	2.16 GHz
DISPlay:SPECtrum:Y[:SCALe]	100 dB
DISPlay:SPECtrum:Y[:SCALe]:OFFSet	0
DISPlay:TDIagram subgroup	
DISPlay:TDIagram:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:TOVerview subgroup	
DISPlay:TOVerview:WINDow:TRACe:GRATICule:GRID:STATe	ON
DISPlay:TOVerview:X[:SCALe]:OFFSet	0
DISPlay:TOVerview:Y[:SCALe]	100 dB
DISPlay:TOVerview:Y[:SCALe]:OFFSet	0

Table C-5: Factory initialization settings, Initiate commands

Header	Default value
INITiate:CONTinuous	ON

Table C-6: Factory initialization settings, Input commands

Header	Default value
INPut[:RF]:ATTenuation	20 dB
INPut[:RF]:ATTenuation:AUTO	ON
INPut[:RF]:ATTenuation:MONitor:STATe	ON
INPut[:RF]:GAIN:STATe	OFF
INPut:{MLEVel RLEVel}	0 dBm

Table C-7: Factory initialization settings, Output commands

Header	Default value
OUTPut:IF:{BANDwidth BWIDTh} (Option 05 only)	FLATtop
OUTPut:IF[:STATe] (Option 05 only)	OFF
OUTPut:IQ[:STATe] (Option 05 only)	OFF
OUTPut:NOISe[:STATe]	OFF

Table C-8: Factory initialization settings, Sense commands

Header	Default value
[SENSe] basic command subgroup	
[SENSe]:ACQuisition:FFRame:LIMit	1
[SENSe]:ACQuisition:FFRame:STATe	OFF
[SENSe]:ACQuisition:MODE	AUTO
[SENSe]:ANALysis:ADVanced:DITHer	AUTO
[SENSe]:ANALysis:LENGth	7.44 μ s
[SENSe]:ANALysis:LENGth:AUTO	ON
[SENSe]:ANALysis:REFerence	ACQSTART
[SENSe]:ANALysis:STARt	0
[SENSe]:ANALysis:STARt:AUTO	ON
[SENSe]:MEASurement:FREQuency:CENTer:LOCK	ON
[SENSe]:POWer:UNITs	DBM
[SENSe]:ROSCillator:SOURce	INTernal
[SENSe]:SPECTrum:LENGth	7.44 μ s

Table C-8: Factory initialization settings, Sense commands (cont.)

Header	Default value
[SENSe]:SPECtrum:LENGth:AUTO	ON
[SENSe]:SPECtrum:STARt	0
[SENSe]:SPECtrum:TIMe:MODE	COMMon
[SENSe]:ACPower subgroup	
[SENSe]:ACPower:AVERage	OFF
[SENSe]:ACPower:AVERage:COUNT	10
[SENSe]:ACPower:{BANDwidth BWIDth}{:RESolution}	30 kHz
[SENSe]:ACPower:{BANDwidth BWIDth}{:RESolution}:AUTO	ON
[SENSe]:ACPower:{BANDwidth BWIDth}:VIDeo	300 kHz
[SENSe]:ACPower:{BANDwidth BWIDth}:VIDeo:STATe	OFF
[SENSe]:ACPower:CHANnel:{BANDwidth BWIDth}	3.84 MHz
[SENSe]:ACPower:CHANnel:FILTer	RRCosine
[SENSe]:ACPower:CHANnel:PAIRs	1
[SENSe]:ACPower:CHANnel:SPACing	5 MHz
[SENSe]:ACPower:CHIPrate	3.84 MHz
[SENSe]:ACPower:FREQuency	1.5 GHz
[SENSe]:ACPower:FREQuency:STEP	1 MHz
[SENSe]:ACPower:FREQuency:STEP:AUTO	ON
[SENSe]:ACPower:NFLoor:STATe	OFF
[SENSe]:ACPower:POINts:COUNT	DRANge
[SENSe]:ACPower:RRCRolloff	0.22
[SENSe]:AM:FM:PM subgroup	
[SENSe]:AM:DETECT:AMPLitude	AVERage
[SENSe]:{AM FM PM}{:MTPoints MAXTracepoints}	HUNDredk
[SENSe]:{FM PM}:BURSt:THReshold	-100 dBc
[SENSe]:{FM PM}:FREQuency:SEARch:AUTO	ON
[SENSe]:PM:PHASe:SEARch:AUTO	ON
[SENSe]:AVTime subgroup	
[SENSe]:AVTime:{BANDwidth BWIDth}	1 MHz
[SENSe]:AVTime:MAXTracepoints	HUNDredk
[SENSe]:AVTime:METHod	SPAN
[SENSe]:AVTime:SPAN	40 MHz
[SENSe]:CCDF subgroup	
[SENSe]:CCDF:{BANDwidth BWIDth}	40 MHz
[SENSe]:CCDF:TIME:TYPE	SINGLE
[SENSe]:DDEMod subgroup	
[SENSe]:DDEMod:ANALysis:LENGth	128 symbols

Table C-8: Factory initialization settings, Sense commands (cont.)

Header	Default value
[SENSe]:DDEMod:ANALysis:LENGth:AUTO	ON
[SENSe]:DDEMod:BURSt:DETECT	OFF
[SENSe]:DDEMod:BURSt:THReshold	-20 dBc
[SENSe]:DDEMod:CARRier:OFFSet	0
[SENSe]:DDEMod:FILTer:ALPHa	0.22
[SENSe]:DDEMod:FILTer:MEASurement	RRCosine
[SENSe]:DDEMod:FILTer:REFerence	RCOSine
[SENSe]:DDEMod:FREQuency:DEViation:AUTO	ON
[SENSe]:DDEMod:MAGNitude:NORMalize	RSYMBOL
[SENSe]:DDEMod:MINDEX	1
[SENSe]:DDEMod:MINDEX:AUTO	ON
[SENSe]:DDEMod:MODulation:TYPE	QPSK
[SENSe]:DDEMod:SRATE	3.84 MHz
[SENSe]:DDEMod:SWAP:IQ	OFF
[SENSe]:DDEMod:SYMBOL:MAP[:STATe]	OFF
[SENSe]:DDEMod:SYMBOL:POINTS	FOUR
[SENSe]:DDEMod:SYNCh:WORD	OFF
[SENSe]:DDEMod:SYNCh:WORD:SYMBOL	#10
[SENSe]:DDEMod:TIME:UNITS	SYMBOLS
[SENSe]:DPSA subgroup	
[SENSe]:DPSA:AUDio:DEMod:GAIN	3
[SENSe]:DPSA:AUDio:DEMod:RXBWidth	30 kHz
[SENSe]:DPSA:AUDio:DEMod:STATe	OFF
[SENSe]:DPSA:AUDio:DEMod:TUNE	SMARker
[SENSe]:DPSA:AUDio:DEMod:TYPE	FM
[SENSe]:DPSA:{BANDwidth BWIDTH}:ACTual?	400 kHz
[SENSe]:DPSA:FREQuency:SPAN:{BANDwidth BWIDTH}[:RESolution]:RATio	ON
[SENSe]:DPSA:COLor	TEMPerature
[SENSe]:DPSA:COLor:MAXimum	100%
[SENSe]:DPSA:POINTs:COUNT	0%
[SENSe]:DPSA:FREQuency:CENTer	1.5 GHz
[SENSe]:DPSA:FREQuency:SPAN	40 MHz
[SENSe]:DPSA:FREQuency:START	1.48 GHz
[SENSe]:DPSA:FREQuency:STEP	2 MHz
[SENSe]:DPSA:FREQuency:STEP:AUTO	ON
[SENSe]:DPSA:FREQuency:STOP	1.52 GHz

Table C-8: Factory initialization settings, Sense commands (cont.)

Header	Default value
[SENSe]:FVTime subgroup	
[SENSe]:FVTime:FREQuency:CENTer	1.5 GHz
[SENSe]:FVTime:FREQuency:SPAN	40 MHz
[SENSe]:FVTime:FREQuency:START	1.48 GHz
[SENSe]:FVTime:FREQuency:STEP	2 MHz
[SENSe]:FVTime:FREQuency:STEP:AUTO	ON
[SENSe]:FVTime:FREQuency:STOP	1.52 GHz
[SENSe]:FVTime:MAXTracepoints	HUNDredk
[SENSe]:IQVTime subgroup	
[SENSe]:IQVTime:FREQuency:CENTer	1.5 GHz
[SENSe]:IQVTime:FREQuency:SPAN	40 MHz
[SENSe]:IQVTime:FREQuency:START	1.48 GHz
[SENSe]:IQVTime:FREQuency:STEP	2 MHz
[SENSe]:IQVTime:FREQuency:STEP:AUTO	ON
[SENSe]:IQVTime:FREQuency:STOP	1.52 GHz
[SENSe]:IQVTime:MAXTracepoints	HUNDredk
[SENSe]:MCPower subgroup	
[SENSe]:MCPower:AVERAge	OFF
[SENSe]:MCPower:AVERAge:COUNT	10
[SENSe]:MCPower:{BANDwidth BWIDth}{:RESolution}	30 kHz
[SENSe]:MCPower:{BANDwidth BWIDth}{:RESolution}:ACTual?	ON
[SENSe]:MCPower:{BANDwidth BWIDth}{:RESolution}:AUTO	300 kHz
[SENSe]:MCPower:{BANDwidth BWIDth}:VIDeo	OFF
[SENSe]:MCPower:{BANDwidth BWIDth}:VIDeo:STATe	3.84 MHz
[SENSe]:MCPower:CHANnel:FILTer	RRCosine
[SENSe]:MCPower:CHANnel:MAIN:{BANDwidth BWIDth}	3.84 MHz
[SENSe]:MCPower:CHANnel:MAIN:COUNT	4
[SENSe]:MCPower:CHANnel:MAIN:INACTive	NONE
[SENSe]:MCPower:CHANnel:MAIN:SPACing	5 MHz
[SENSe]:MCPower:CHIPrate	3.84 MHz
[SENSe]:MCPower:FREQuency	1.5 GHz
[SENSe]:MCPower:FREQuency:STEP	2 MHz
[SENSe]:MCPower:FREQuency:STEP:AUTO	ON
[SENSe]:MCPower:NFLoor:STATe	OFF
[SENSe]:MCPower:POINts:COUNT	DRANge
[SENSe]:MCPower:RRCRolloff	0.22
[SENSe]:OBWidth subgroup	

Table C-8: Factory initialization settings, Sense commands (cont.)

Header	Default value
[SENSe]:OBWidth:AVERage	OFF
[SENSe]:OBWidth:AVERage:COUNT	10
[SENSe]:OBWidth:{BANDwidth BWIDth}:MEASurement	10 MHz
[SENSe]:OBWidth:{BANDwidth BWIDth}[:RESolution]	33 kHz
[SENSe]:OBWidth:{BANDwidth BWIDth}[:RESolution]:AUTO	ON
[SENSe]:OBWidth:{BANDwidth BWIDth}:VIDeo	300 kHz
[SENSe]:OBWidth:{BANDwidth BWIDth}:VIDeo:STATe	OFF
[SENSe]:OBWidth:FREQuency:CENTer	1.5 GHz
[SENSe]:OBWidth:FREQuency:STEP	2 MHz
[SENSe]:OBWidth:FREQuency:STEP:AUTO	ON
[SENSe]:OBWidth:PERCent	99%
[SENSe]:OBWidth:XDBLevel	-26 dB
[SENSe]:PHVTime subgroup	
[SENSe]:PHVTime:FREQuency:CENTer	1.5 GHz
[SENSe]:PHVTime:FREQuency:SPAN	40 MHz
[SENSe]:PHVTime:FREQuency:STARt	1.48 GHz
[SENSe]:PHVTime:FREQuency:STEP	2 MHz
[SENSe]:PHVTime:FREQuency:STEP:AUTO	ON
[SENSe]:PHVTime:FREQuency:STOP	1.52 GHz
[SENSe]:PHVTime:MAXTracepoints	HUNDredk
[SENSe]:PNOise subgroup	
[SENSe]:PNOise:AVERage:COUNT	10
[SENSe]:PNOise:AVERage:ENABle	OFF
[SENSe]:PNOise:CARRier:FREQuency:TRACk	ON
[SENSe]:PNOise:CARRier:THReshold	-26 dBm
[SENSe]:PNOise:FREQuency:INTegration:OFFSet:STARt	100 Hz
[SENSe]:PNOise:FREQuency:INTegration:OFFSet:STOP	10 MHz
[SENSe]:PNOise:FREQuency:PLOT:OFFSet:STARt	10 Hz
[SENSe]:PNOise:FREQuency:PLOT:OFFSet:STOP	100 MHz
[SENSe]:PNOise:OPTimization	SPEed
[SENSe]:PULSe subgroup	
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:ALENgtH	1e-6
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:METHod	RELative
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:RLENgtH	100
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:RLEVel	100
[SENSe]:PULSe:ANALyze:FDOMain:MEASurement:TIME:STARt	0

Table C-8: Factory initialization settings, Sense commands (cont.)

Header	Default value
[SENSe]:PULSe:ANALyze:IRESpOse:CORRection:AMPLitude[:STATe]	ON
[SENSe]:PULSe:ANALyze:IRESpOse:KOTime	0
[SENSe]:PULSe:ANALyze:IRESpOse:MEASurement:TIME:ALENgtH	1e-6
[SENSe]:PULSe:ANALyze:IRESpOse:MEASurement:TIME:METhod	RELative
[SENSe]:PULSe:ANALyze:IRESpOse:MEASurement:TIME:RLENgtH	100
[SENSe]:PULSe:ANALyze:IRESpOse:MEASurement:TIME:RLEVel	100
[SENSe]:PULSe:ANALyze:IRESpOse:MEASurement:TIME:STARt	0
[SENSe]:PULSe:ANALyze:LEVel	VOLTage
[SENSe]:PULSe:ANALyze:LEVel:FIFTy	VOLTage
[SENSe]:PULSe:ANALyze:LEVel:HUNDred	AVERage
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:ALENgtH	1e-6
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:METhod	RELative
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLENgtH	25
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:RLEVel	100
[SENSe]:PULSe:ANALyze:OVERshoot:MEASurement:TIME:STARt	0
[SENSe]:PULSe:ANALyze:PMLocation	500 ns
[SENSe]:PULSe:ANALyze:POINt:LOCation	AVERage
[SENSe]:PULSe:ANALyze:RFALI	WIDE
[SENSe]:PULSe:ANALyze:RIPPlE	50%
[SENSe]:PULSe:CARRier:SEARCh	AUTO
[SENSe]:PULSe:DETEct:MEASurement	OFF
[SENSe]:PULSe:DETEct:NUMBer	100
[SENSe]:PULSe:DETEct:POWer[:THReshold]	-10 dBc
[SENSe]:PULSe:DETEct:TIME[:THReshold]	1 ns
[SENSe]:PULSe:FILTer:{BANDwidth BWIDTH}	20 MHz (Standard), 60 MHz (Option 110)
[SENSe]:PULSe:FILTer:MEASurement	GAUSSian
[SENSe]:PULSe:FREFerence:AUTO	ON
[SENSe]:PULSe:FREFerence:CSLope:AUTO	ON
[SENSe]:PULSe:FREFerence:OFFSet	0
[SENSe]:PULSe:MODulation:TYPE	CWConst
[SENSe]:PULSe:STATistics:HISTogram:ORDinate	COUNT
[SENSe]:PULSe:STATistics:HISTogram:POINts:AUTO	ON
[SENSe]:REANalyze:NEXT	CWConst
[SENSe]:SGRam subgroup	

Table C-8: Factory initialization settings, Sense commands (cont.)

Header	Default value
[SENSe]:SGRam:{BANDwidth BWIDth}:OPTimization	AUTO
[SENSe]:SGRam:{BANDwidth BWIDth}:RESolution	300 kHz
[SENSe]:SGRam:{BANDwidth BWIDth}[:RESolution]:AUTO	ON
[SENSe]:SGRam:{BANDwidth BWIDth}[:RESolution]:MODE	ON
[SENSe]:SGRam:{BANDwidth BWIDth}:VIDeo	300 kHz
[SENSe]:SGRam:{BANDwidth BWIDth}:VIDeo:STATe	OFF
[SENSe]:SGRam:COLor	TEMPerature
[SENSe]:SGRam:COLor:MAXimum	0 dBm
[SENSe]:SGRam:COLor:MINimum	-100 dBm
[SENSe]:SGRam:FFT:WINDow	KAISer
[SENSe]:SGRam:FILTer[:SHAPE]	KAISer
[SENSe]:SGRam:FREQuency:CENTer	1.5 GHz
[SENSe]:SGRam:FREQuency:SPAN	40 MHz
[SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:RESolution]:RATio	100
[SENSe]:SGRam:FREQuency:START	1.48 GHz
[SENSe]:SGRam:FREQuency:STEP	2 MHz
[SENSe]:SGRam:FREQuency:STEP:AUTO	ON
[SENSe]:SGRam:FREQuency:STOP	1.52 GHz
[SENSe]:SPECTrum subgroup	
[SENSe]:SPECTrum:{BANDwidth BWIDth}:OPTimization	AUTO
[SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]	300 kHz
[SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]:AUTO	ON
[SENSe]:SPECTrum:{BANDwidth BWIDth}[:RESolution]:MODE	ON
[SENSe]:SPECTrum:{BANDwidth BWIDth}:VIDeo	300 kHz
[SENSe]:SPECTrum:{BANDwidth BWIDth}:VIDeo:STATe	OFF
[SENSe]:SPECTrum:FFT:WINDow	KAISer
[SENSe]:SPECTrum:FILTer[:SHAPE]	KAISer
[SENSe]:SPECTrum:FREQuency:CENTer	1.5 GHz
[SENSe]:SPECTrum:FREQuency:SPAN	40 MHz
[SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio	100
[SENSe]:SPECTrum:FREQuency:START	1.48 GHz
[SENSe]:SPECTrum:FREQuency:STEP	2 MHz
[SENSe]:SPECTrum:FREQuency:STEP:AUTO	ON
[SENSe]:SPECTrum:FREQuency:STOP	1.52 GHz
[SENSe]:SPECTrum:POINTs:COUNT	P801
[SENSe]:SPURious subgroup	

Table C-8: Factory initialization settings, Sense commands (cont.)

Header	Default value
[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}	4 MHz
[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}:INTEgration	1 MHz
[SENSe]:SPURious:CARRier:{BANDwidth BWIDth}[:RESolution]: AUTO	ON
[SENSe]:SPURious:CARRier:DETEction	PEAK
[SENSe]:SPURious:CARRier:FREQUency	1.484 GHz
[SENSe]:SPURious:CARRier:THReshold	-10 dBm
[SENSe]:SPURious:LIST	OVERlimit
[SENSe]:SPURious:MODE	MULTi
[SENSe]:SPURious:OPTimization	AUTO
[SENSe]:SPURious:POINts:COUNT	P801
[SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo	300 kHz
[SENSe]:SPURious:RANGe<x>:BANDwidth:VIDeo:STATe	OFF
[SENSe]:SPURious:RANGe<x>:DETEction	PEAK
[SENSe]:SPURious:RANGe<x>:EXCURsion	6 dB
[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPe]	RBW
[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPe]:BANDwidth	200 kHz
[SENSe]:SPURious:RANGe<x>:FILTer[:SHAPe]:BANDwidth:AUTO	ON
[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:START	-50 dBm
[SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:STOP	-50 dBm
[SENSe]:SPURious:RANGe<x>:LIMit:MASK	ABS
[SENSe]:SPURious:RANGe<x>:LIMit:RELAtive:START	-30 dB
[SENSe]:SPURious:RANGe<x>:LIMit:RELAtive:STOP	-30 dB
[SENSe]:SPURious:RANGe<x>:STATe	<x>=1: ON <x>=2 to 20: OFF
[SENSe]:SPURious:REFerence	NONE
[SENSe]:SPURious:REFerence:MANual:POWer	-10 dBm
[SENSe]:TOVerview subgroup	
[SENSe]:TOVerview:FREQUency:CENTer	1.5 GHz
[SENSe]:TOVerview:MAXTracepoints	HUNDredk

Table C-9: Factory initialization settings, Trace commands

Header	Default value
TRACe:{AM FM PM} subgroup	
TRACe:{AM FM PM}	ON
TRACe<x>:AVTime:DETEction	POSitive

Table C-9: Factory initialization settings, Trace commands (cont.)

Header	Default value
TRACe:{AM FM PM}:FREeze	OFF
TRACe:{AM FM PM}:FUNction	NORMal
TRACe<x>:AVTime subgroup	
TRACe<x>:AVTime	<x>=1: ON <x>=2 to 4: OFF
TRACe<x>:AVTime:AVERAge:COUNT	10
TRACe<x>:AVTime:COUNT	10
TRACe<x>:AVTime:COUNT:ENABLE	ON
TRACe<x>:AVTime:FREeze	OFF
TRACe<x>:AVTime:FUNction	NORMal
TRACe<x>:AVTime:LEFTooperand	TRACE2
TRACe<x>:AVTime:RIGHTooperand	TRACE1
TRACe<x>:CCDF subgroup	
TRACe<x>:CCDF:FREeze	OFF
TRACe<x>:CCDF:SHOW	<x>=1: ON <x>=2 and 3: OFF
TRACe<x>:CCDF:X	3 dB
TRACe:CONStE subgroup	
TRACe:CONStE:MODE	VECTors
TRACe:DIQVtime subgroup	
TRACe:DIQVtime:ENABLE:I	ON
TRACe:DIQVtime:ENABLE:Q	ON
TRACe<x>:DPSA subgroup	
TRACe<x>:DPSA	<x>=1 and 5: ON <x>=2 to 4: OFF
TRACe<x>:DPSA:AVERAge:COUNT	10
TRACe<x>:DPSA:COLor:CURVe	25 %
TRACe<x>:DPSA:DOT:PERStent	(<x>=5 only) ON
TRACe<x>:DPSA:DOT:PERStent:TYPE	(<x>=5 only) VARiable
TRACe<x>:DPSA:DOT:PERStent:VARiable	(<x>=5 only) 10
TRACe<x>:DPSA:FREeze	OFF
TRACe<x>:DPSA:DETEction	NORMal
TRACe<x>:DPSA:LEFTooperand	TRACE1
TRACe<x>:DPSA:RIGHTooperand	TRACE3
TRACe:EDlagram subgroup	
TRACe:EDlagram:ENABLE:I	ON
TRACe:EDlagram:ENABLE:Q	ON

Table C-9: Factory initialization settings, Trace commands (cont.)

Header	Default value
TRACe:FVTime subgroup	
TRACe:FVTime:COUNT	10
TRACe:FVTime:COUNT:ENABle	ON
TRACe:FVTime:FREeze	OFF
TRACe:FVTime:FUNCTioN	NORMal
TRACe:IQVTime subgroup	
TRACe:IQVTime:COUNT	10
TRACe:IQVTime:DETECTioN	ON
TRACe:IQVTime:ENABle:I	ON
TRACe:IQVTime:ENABle:Q	ON
TRACe:IQVTime:FREeze	OFF
TRACe:IQVTime:FUNCTioN	NORMal
TRACe:IQVTime:SElect:I	ON
TRACe:IQVTime:SElect:Q	OFF
TRACe:OBWidth subgroup	
TRACe:OBW:MAXHold	OFF
TRACe:PHVTime subgroup	
TRACe:PHVTime:COUNT	10
TRACe:PHVTime:COUNT:ENABle	ON
TRACe:PHVTime:FREeze	OFF
TRACe:PHVTime:FUNCTioN	NORMal
TRACe<x>:PNOise subgroup	
TRACe<x>:PNOise:SHOW	<x>=1: ON <x>=2: OFF
TRACe<x>:PNOise:SMOothing:COUNT	5
TRACe<x>:PNOise:SMOothing:ENABle	ON
TRACe:SGRam subgroup	
TRACe<x>:PHVTime:DETECTioN	POSitive
TRACe:SGRam:FREeze	OFF
TRACe:SGRam:FUNCTioN	NONE
TRACe:SGRam:FUNCTioN:TIME	0.02 minutes
TRACe:SGRam:SElect:LINE	0
TRACe<x>:SPECTrum subgroup	
TRACe<x>:SPECTrum	<x>=1: ON <x>=2 to 4: OFF
TRACe<x>:SPECTrum:AVERAge:COUNT	10
TRACe<x>:SPECTrum:COUNT	10

Table C-9: Factory initialization settings, Trace commands (cont.)

Header	Default value
TRACe<x>:SPECtrum:COUNT:ENABLE	ON
TRACe<x>:SPECtrum:DETection	POSitive
TRACe<x>:SPECtrum:FREeze	OFF
TRACe<x>:SPECtrum:FUNcTion	NONE
TRACe<x>:SPECtrum:LEFTooperand	TRACE2
TRACe<x>:SPECtrum:RIGHTooperand	TRACE1
TRACe:SPURious subgroup	
TRACe:SPURious:COUNT	10
TRACe:SPURious:COUNT:ENABLE	ON
TRACe1:TOVerview:COUNT:RESet	OFF
TRACe:SPURious:FUNcTion	NONE

Table C-10: Factory initialization settings, Trigger commands

Header	Default value
TRIGger:DPSA:SHOW:FRAMES	OFF
TRIGger[:SEQuence]:EVENT:EXTFront:IMPedance	5 k Ω
TRIGger[:SEQuence]:EVENT:EXTFront:LEVel	1.6 V
TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe	RISe
TRIGger[:SEQuence]:EVENT:GATed	HIGH
TRIGger[:SEQuence]:EVENT:INPut:FMASK:BANDwidth BWIDTH[:RESolution]:ACTual?	FT
TRIGger[:SEQuence]:EVENT:INPut:DDENsity:AMPLitude:TOLerance	-20 dBm
TRIGger[:SEQuence]:EVENT:INPut:RUNT:PULse:HIGH:LEVel	-10 dBm
TRIGger[:SEQuence]:EVENT:INPut:TDBWidth	1 MHz
TRIGger[:SEQuence]:EVENT:INPut:TDBWidth:STATe	ON
TRIGger[:SEQuence]:EVENT:INPut:TYPE	POWer
TRIGger[:SEQuence]:EVENT:SOURce	INPut
TRIGger[:SEQuence]:FORCed	OFF
TRIGger[:SEQuence]:TIME:QUALified:TIME<x>	OFF
TRIGger[:SEQuence]:ADVanced:HOLDoff:ENABLE	0 s
TRIGger[:SEQuence]:TIME:POSition	25%

Table C-11: Factory initialization settings, UNIT commands

Header	Default value
UNIT:POWer	dBm

Appendix D: SCPI Conformance Information

All commands for the RSA6100A Series analyzers are based on SCPI Version 1999.0. The following table lists the commands that are defined in the SCPI 1999.0 Standard. The other commands not listed in the table are not defined in the SCPI 1999.0 Standard.

Table D-1: SCPI 1999.0-defined commands

Command group	Command			
IEEE common	*CAL			
	*CLS			
	*ESE			
	*ESR			
	*IDN			
	*OPC			
	*OPT			
	*RST			
	*SRE			
	*STB			
	*TRG			
	*WAI			
ABORT	:ABORT			
INITiate	:INITiate	:CONTinuous		
		[:IMMediate]		
STATus	:STATus	:OPERation	:CONDition?	
			:ENABle	
		[:EVENT]?		
		:NTRansition		
		:PTRansition		
		:PRESet		
		:QUESTionable	:CONDition?	
			:ENABle	
			[:EVENT]?	
			:NTRansition	
:PTRansition				

Table D-1: SCPI 1999.0-defined commands (cont.)

Command group	Command	
SYSTEM	:SYSTEM :COMMunicate :GPIB [:SELF] :ADDRESS	
	:DATE	
	:ERRor :ALL?	
	:CODE :ALL?	
	:NEXT?	
	:COUNT?	
	:NEXT?	
	:PRESet	
	:TIME	
	:VERSion?	
	UNIT	:UNIT :POWER

Glossary

Glossary

ASCII

Acronym for the American Standard Code for Information Interchange. Controllers transmit commands to the instrument using ASCII character encoding.

ASK

Acronym for Amplitude Shift Keying. The process, or result of a process, in which the amplitude of the carrier is varied in accordance with the state of a digital input signal.

BNF (Backus-Naur Form)

A standard notation system for command syntax diagrams. The syntax diagrams in this manual use BNF notation.

Controller

A computer or other device that sends commands to and accepts responses from the analyzer.

EVM (Error Vector Magnitude)

The magnitude of an error of an actual signal relative to an ideal signal in a constellation display.

GPIB

Acronym for General Purpose Interface Bus, the common name for the communications interface system defined in IEEE Std 488.

IEEE

Acronym for the Institute for Electrical and Electronic Engineers.

IS95

Acronym for Interim Standard-95. The standards name for first-generation CDMA cellphone technology.

Modulation

The process of varying some characteristic of a signal with a second signal.

PSK

Acronym for Phase Shift Keying. The process, or result of a process, in which the carrier phase is varied discretely in accordance with a digital code.

QAM

Acronym for Quadrature Amplitude Modulation. The process, or result of a process, in which the amplitude and phase of the carrier are varied concurrently by synthesizing two orthogonal ASK waves (see ASK).

Index

A

ABORt, 2-81

C

*CAL, 2-81

Calculate Commands, 2-16

CALCulate:{AM|FM|PM}:MARKer<x>:DELTA:
X?, 2-85

CALCulate:{AM|FM|PM}:MARKer<x>:DELTA:
Y?, 2-86

CALCulate:{AM|FM|PM}:MARKer<x>:
MAXimum, 2-87

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:
HIGHer, 2-87

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:
LEFT, 2-88

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:
LOWer, 2-88

CALCulate:{AM|FM|PM}:MARKer<x>:PEAK:
RIGHT, 2-89

CALCulate:{AM|FM|PM}:MARKer<x>:X, 2-89

CALCulate:{AM|FM|PM}:MARKer<x>:Y?, 2-90

CALCulate:ACPower:MARKer<x>:DELTA:X?, 2-82

CALCulate:ACPower:MARKer<x>:DELTA:Y?, 2-82

CALCulate:ACPower:MARKer<x>:MAXimum, 2-83

CALCulate:ACPower:MARKer<x>:PEAK:
LEFT, 2-83

CALCulate:ACPower:MARKer<x>:PEAK:
RIGHT, 2-84

CALCulate:ACPower:MARKer<x>:X, 2-84

CALCulate:ACPower:MARKer<x>:Y?, 2-85

CALCulate:AVTime:MARKer<x>:DELTA:X?, 2-90

CALCulate:AVTime:MARKer<x>:DELTA:Y?, 2-91

CALCulate:AVTime:MARKer<x>:MAXimum, 2-91

CALCulate:AVTime:MARKer<x>:PEAK:
HIGHer, 2-92

CALCulate:AVTime:MARKer<x>:PEAK:LEFT, 2-92

CALCulate:AVTime:MARKer<x>:PEAK:
LOWer, 2-93

CALCulate:AVTime:MARKer<x>:PEAK:
RIGHT, 2-93

CALCulate:AVTime:MARKer<x>:TRACe, 2-94

CALCulate:AVTime:MARKer<x>:X, 2-94

CALCulate:AVTime:MARKer<x>:Y?, 2-95

CALCulate:CONStE:MARKer<x>:DELTA:X[:
TIME]?, 2-95

CALCulate:CONStE:MARKer<x>:FDEVIation?, 2-96

CALCulate:CONStE:MARKer<x>:
MAGNitude?, 2-97

CALCulate:CONStE:MARKer<x>:MAXimum, 2-97

CALCulate:CONStE:MARKer<x>:PEAK:LEFT, 2-98

CALCulate:CONStE:MARKer<x>:PEAK:
RIGHT, 2-98

CALCulate:CONStE:MARKer<x>:PHASe?, 2-99

CALCulate:CONStE:MARKer<x>:SYMBOL?, 2-100

CALCulate:CONStE:MARKer<x>:VALue?, 2-100

CALCulate:CONStE:MARKer<x>:X, 2-101

CALCulate:DIQVtime:MARKer<x>:DELTA:X[:
TIME]?, 2-101

CALCulate:DIQVtime:MARKer<x>:DELTA:
Y?, 2-102

CALCulate:DIQVtime:MARKer<x>:
MAXimum, 2-103

CALCulate:DIQVtime:MARKer<x>:PEAK:
HIGHer, 2-103

CALCulate:DIQVtime:MARKer<x>:PEAK:
LEFT, 2-104

CALCulate:DIQVtime:MARKer<x>:PEAK:
LOWer, 2-104

CALCulate:DIQVtime:MARKer<x>:PEAK:
RIGHT, 2-105

CALCulate:DIQVtime:MARKer<x>:TRACe, 2-105

CALCulate:DIQVtime:MARKer<x>:X[:
TIME], 2-106

CALCulate:DIQVtime:MARKer<x>:Y?, 2-107

CALCulate:DPSA:MARKer<x>:DELTA:X:
AMPLitude?, 2-107

CALCulate:DPSA:MARKer<x>:DELTA:X[:
FREQuency]?, 2-108

CALCulate:DPSA:MARKer<x>:DELTA:Y?, 2-109

CALCulate:DPSA:MARKer<x>:MAXimum, 2-109

CALCulate:DPSA:MARKer<x>:PEAK:
HIGHer, 2-110

CALCulate:DPSA:MARKer<x>:PEAK:LEFT, 2-110

CALCulate:DPSA:MARKer<x>:PEAK:
LOWer, 2-111

CALCulate:DPSA:MARKer<x>:PEAK:RIGHT, 2-111

- CALCulate:DPSA:MARKer<x>:TRACe, 2-112
CALCulate:DPSA:MARKer<x>:X:
 AMPLitude, 2-113
CALCulate:DPSA:MARKer<x>:X[:
 FREQuency], 2-114
CALCulate:DPSA:MARKer<x>:Y?, 2-114
CALCulate:DPSA:MARKer<x>[:SET]:
 CENTer, 2-112
CALCulate:EDIagram:MARKer<x>:DELTA:X[:
 TIME]?, 2-115
CALCulate:EDIagram:MARKer<x>:DELTA:
 Y?, 2-116
CALCulate:EDIagram:MARKer<x>:
 MAXimum, 2-116
CALCulate:EDIagram:MARKer<x>:PEAK:
 HIGHer, 2-117
CALCulate:EDIagram:MARKer<x>:PEAK:
 LEFT, 2-117
CALCulate:EDIagram:MARKer<x>:PEAK:
 LOWer, 2-118
CALCulate:EDIagram:MARKer<x>:PEAK:
 RIGHT, 2-118
CALCulate:EDIagram:MARKer<x>:TRACe, 2-119
CALCulate:EDIagram:MARKer<x>:X[:
 TIME], 2-120
CALCulate:EDIagram:MARKer<x>:Y?, 2-120
CALCulate:EVM:MARKer<x>:DELTA:X?, 2-121
CALCulate:EVM:MARKer<x>:DELTA:Y?, 2-121
CALCulate:EVM:MARKer<x>:MAXimum, 2-122
CALCulate:EVM:MARKer<x>:PEAK:
 HIGHer, 2-123
CALCulate:EVM:MARKer<x>:PEAK:LEFT, 2-123
CALCulate:EVM:MARKer<x>:PEAK:LOWer, 2-124
CALCulate:EVM:MARKer<x>:PEAK:RIGHT, 2-124
CALCulate:EVM:MARKer<x>:X, 2-125
CALCulate:EVM:MARKer<x>:Y?, 2-125
CALCulate:FDVTime:MARKer<x>:DELTA:X[:
 TIME]?, 2-126
CALCulate:FDVTime:MARKer<x>:DELTA:
 Y?, 2-127
CALCulate:FDVTime:MARKer<x>:
 MAXimum, 2-127
CALCulate:FDVTime:MARKer<x>:PEAK:
 HIGHer, 2-128
CALCulate:FDVTime:MARKer<x>:PEAK:
 LEFT, 2-128
CALCulate:FDVTime:MARKer<x>:PEAK:
 LOWer, 2-129
CALCulate:FDVTime:MARKer<x>:PEAK:
 RIGHT, 2-129
CALCulate:FDVTime:MARKer<x>:X[:TIME], 2-130
CALCulate:FDVTime:MARKer<x>:Y?, 2-130
CALCulate:FVTime:MARKer<x>:DELTA:X?, 2-131
CALCulate:FVTime:MARKer<x>:DELTA:Y?, 2-131
CALCulate:FVTime:MARKer<x>:MAXimum, 2-132
CALCulate:FVTime:MARKer<x>:PEAK:
 HIGHer, 2-132
CALCulate:FVTime:MARKer<x>:PEAK:
 LEFT, 2-133
CALCulate:FVTime:MARKer<x>:PEAK:
 LOWer, 2-133
CALCulate:FVTime:MARKer<x>:PEAK:
 RIGHT, 2-134
CALCulate:FVTime:MARKer<x>:X, 2-134
CALCulate:FVTime:MARKer<x>:Y?, 2-135
CALCulate:IQVTime:MARKer<x>:DELTA:X?, 2-136
CALCulate:IQVTime:MARKer<x>:DELTA:Y?, 2-136
CALCulate:IQVTime:MARKer<x>:
 MAXimum, 2-137
CALCulate:IQVTime:MARKer<x>:PEAK:
 HIGHer, 2-137
CALCulate:IQVTime:MARKer<x>:PEAK:
 LEFT, 2-138
CALCulate:IQVTime:MARKer<x>:PEAK:
 LOWer, 2-138
CALCulate:IQVTime:MARKer<x>:PEAK:
 RIGHT, 2-139
CALCulate:IQVTime:MARKer<x>:TRACe, 2-139
CALCulate:IQVTime:MARKer<x>:X, 2-140
CALCulate:IQVTime:MARKer<x>:Y?, 2-140
CALCulate:MARKer:ADD, 2-141
CALCulate:MARKer:AOff, 2-141
CALCulate:MARKer:DELEte, 2-142
CALCulate:MARKer:DENSity:EXCursion, 2-142
CALCulate:MARKer:DENSity:SMOothing, 2-143
CALCulate:MARKer:DENSity:THREshold, 2-144
CALCulate:MARKer:MODE, 2-144
CALCulate:MARKer:PEAK:EXCursion, 2-145
CALCulate:MARKer:PEAK:THREshold, 2-145
CALCulate:MCPower:MARKer<x>:DELTA:
 X?, 2-146
CALCulate:MCPower:MARKer<x>:DELTA:
 Y?, 2-146

- CALCulate:MCPower:MARKer<x>:
MAXimum, 2-147
- CALCulate:MCPower:MARKer<x>:PEAK:
LEFT, 2-147
- CALCulate:MCPower:MARKer<x>:PEAK:
RIGHT, 2-148
- CALCulate:MCPower:MARKer<x>:X, 2-148
- CALCulate:MCPower:MARKer<x>:Y?, 2-149
- CALCulate:MERRor:MARKer<x>:DELTA:X?, 2-149
- CALCulate:MERRor:MARKer<x>:DELTA:Y?, 2-150
- CALCulate:MERRor:MARKer<x>:
MAXimum, 2-151
- CALCulate:MERRor:MARKer<x>:PEAK:
HIGHer, 2-151
- CALCulate:MERRor:MARKer<x>:PEAK:
LEFT, 2-152
- CALCulate:MERRor:MARKer<x>:PEAK:
LOWer, 2-152
- CALCulate:MERRor:MARKer<x>:PEAK:
RIGHT, 2-153
- CALCulate:MERRor:MARKer<x>:X, 2-153
- CALCulate:MERRor:MARKer<x>:Y?, 2-154
- CALCulate:OBWidth:MARKer<x>:DELTA:X?, 2-154
- CALCulate:OBWidth:MARKer<x>:DELTA:Y?, 2-155
- CALCulate:OBWidth:MARKer<x>:
MAXimum, 2-156
- CALCulate:OBWidth:MARKer<x>:PEAK:
HIGHer, 2-156
- CALCulate:OBWidth:MARKer<x>:PEAK:
LEFT, 2-157
- CALCulate:OBWidth:MARKer<x>:PEAK:
LOWer, 2-157
- CALCulate:OBWidth:MARKer<x>:PEAK:
RIGHT, 2-158
- CALCulate:OBWidth:MARKer<x>:X, 2-159
- CALCulate:OBWidth:MARKer<x>:Y?, 2-159
- CALCulate:OBWidth:MARKer<x>[:SET]:
CENTer, 2-158
- CALCulate:PERRor:MARKer<x>:DELTA:X?, 2-160
- CALCulate:PERRor:MARKer<x>:DELTA:Y?, 2-160
- CALCulate:PERRor:MARKer<x>:MAXimum, 2-161
- CALCulate:PERRor:MARKer<x>:PEAK:
HIGHer, 2-161
- CALCulate:PERRor:MARKer<x>:PEAK:
LEFT, 2-162
- CALCulate:PERRor:MARKer<x>:PEAK:
LOWer, 2-162
- CALCulate:PERRor:MARKer<x>:PEAK:
RIGHT, 2-163
- CALCulate:PERRor:MARKer<x>:X, 2-163
- CALCulate:PERRor:MARKer<x>:Y?, 2-164
- CALCulate:PHVTime:MARKer<x>:DELTA:
X?, 2-164
- CALCulate:PHVTime:MARKer<x>:DELTA:
Y?, 2-165
- CALCulate:PHVTime:MARKer<x>:
MAXimum, 2-166
- CALCulate:PHVTime:MARKer<x>:PEAK:
HIGHer, 2-166
- CALCulate:PHVTime:MARKer<x>:PEAK:
LEFT, 2-167
- CALCulate:PHVTime:MARKer<x>:PEAK:
LOWer, 2-167
- CALCulate:PHVTime:MARKer<x>:PEAK:
RIGHT, 2-168
- CALCulate:PHVTime:MARKer<x>:X, 2-168
- CALCulate:PHVTime:MARKer<x>:Y?, 2-169
- CALCulate:PULSe:STATistics:FFT:INDicator:
X, 2-169
- CALCulate:PULSe:STATistics:FFT:INDicator:
Y?, 2-170
- CALCulate:PULSe:STATistics:HISTogram:
INDicator:X, 2-170
- CALCulate:PULSe:STATistics:HISTogram:
INDicator:Y?, 2-171
- CALCulate:PULSe:STATistics:MARKer<x>:DELTA:
X?, 2-171
- CALCulate:PULSe:STATistics:MARKer<x>:DELTA:
Y?, 2-172
- CALCulate:PULSe:STATistics:MARKer<x>:
MAXimum, 2-172
- CALCulate:PULSe:STATistics:MARKer<x>:PEAK:
HIGHer, 2-173
- CALCulate:PULSe:STATistics:MARKer<x>:PEAK:
LEFT, 2-173
- CALCulate:PULSe:STATistics:MARKer<x>:PEAK:
LOWer, 2-174
- CALCulate:PULSe:STATistics:MARKer<x>:PEAK:
RIGHT, 2-174
- CALCulate:PULSe:STATistics:MARKer<x>:
X, 2-175
- CALCulate:PULSe:STATistics:MARKer<x>:
Y?, 2-175

- CALCulate:PULSe:TRACe:MARKer<x>:DELTA:
X?, 2-176
- CALCulate:PULSe:TRACe:MARKer<x>:DELTA:
Y?, 2-177
- CALCulate:PULSe:TRACe:MARKer<x>:
MAXimum, 2-177
- CALCulate:PULSe:TRACe:MARKer<x>:PEAK:
HIGHer, 2-178
- CALCulate:PULSe:TRACe:MARKer<x>:PEAK:
LEFT, 2-178
- CALCulate:PULSe:TRACe:MARKer<x>:PEAK:
LOWer, 2-179
- CALCulate:PULSe:TRACe:MARKer<x>:PEAK:
RIGHT, 2-179
- CALCulate:PULSe:TRACe:MARKer<x>:X, 2-180
- CALCulate:PULSe:TRACe:MARKer<x>:Y?, 2-180
- CALCulate:SEARch:LIMit:FAIL?, 2-181
- CALCulate:SEARch:LIMit:MATCH:BEEP[:
STATE], 2-181
- CALCulate:SEARch:LIMit:MATCH:SACQuire[:
STATE], 2-182
- CALCulate:SEARch:LIMit:MATCH:SDATa[:
STATE], 2-182
- CALCulate:SEARch:LIMit:MATCH:SPICture[:
STATE], 2-183
- CALCulate:SEARch:LIMit:MATCH:STRace[:
STATE], 2-184
- CALCulate:SEARch:LIMit:OPERation, 2-184
- CALCulate:SEARch:LIMit:OPERation:FEED, 2-185
- CALCulate:SEARch:LIMit:OPERation:MASK:
LOAD, 2-186
- CALCulate:SEARch:LIMit:OPERation:MASK:
STORE, 2-187
- CALCulate:SEARch:LIMit:OPERation:
SLIMit, 2-187
- CALCulate:SEARch:LIMit:REPort:DATA?, 2-188
- CALCulate:SEARch:LIMit:REPort:POINts?, 2-188
- CALCulate:SEARch:LIMit:STATE, 2-189
- CALCulate:SGRam:MARKer<x>:DELTA:X:
FREQuency?, 2-189
- CALCulate:SGRam:MARKer<x>:DELTA:X[:
TIME]?, 2-190
- CALCulate:SGRam:MARKer<x>:DELTA:Y?, 2-190
- CALCulate:SGRam:MARKer<x>:MAXimum, 2-191
- CALCulate:SGRam:MARKer<x>:PEAK:
HIGHer, 2-191
- CALCulate:SGRam:MARKer<x>:PEAK:
LEFT, 2-192
- CALCulate:SGRam:MARKer<x>:PEAK:
LOWer, 2-192
- CALCulate:SGRam:MARKer<x>:PEAK:
RIGHT, 2-193
- CALCulate:SGRam:MARKer<x>:X:
FREQuency, 2-194
- CALCulate:SGRam:MARKer<x>:X[:TIME], 2-194
- CALCulate:SGRam:MARKer<x>:Y?, 2-195
- CALCulate:SGRam:MARKer<x>[:SET]:
CENTer, 2-193
- CALCulate:SPECtrum:MARKer<x>:DELTA:
X?, 2-195
- CALCulate:SPECtrum:MARKer<x>:DELTA:
Y?, 2-196
- CALCulate:SPECtrum:MARKer<x>:
MAXimum, 2-197
- CALCulate:SPECtrum:MARKer<x>:PEAK:
HIGHer, 2-197
- CALCulate:SPECtrum:MARKer<x>:PEAK:
LEFT, 2-197
- CALCulate:SPECtrum:MARKer<x>:PEAK:
LOWer, 2-198
- CALCulate:SPECtrum:MARKer<x>:PEAK:
RIGHT, 2-198
- CALCulate:SPECtrum:MARKer<x>:TRACe, 2-199
- CALCulate:SPECtrum:MARKer<x>:X, 2-200
- CALCulate:SPECtrum:MARKer<x>:Y?, 2-201
- CALCulate:SPECtrum:MARKer<x>[:SET]:
CENTer, 2-199
- CALCulate:SPURious:MARKer<x>:DELTA:
X?, 2-201
- CALCulate:SPURious:MARKer<x>:DELTA:
Y?, 2-202
- CALCulate:SPURious:MARKer<x>:
MAXimum, 2-202
- CALCulate:SPURious:MARKer<x>:PEAK:
HIGHer, 2-203
- CALCulate:SPURious:MARKer<x>:PEAK:
LEFT, 2-203
- CALCulate:SPURious:MARKer<x>:PEAK:
LOWer, 2-204
- CALCulate:SPURious:MARKer<x>:PEAK:
RIGHT, 2-204
- CALCulate:SPURious:MARKer<x>:X, 2-205
- CALCulate:SPURious:MARKer<x>:Y?, 2-205

CALCulate:SPURious:MARKer<x>[:SET]:
 CENTer, 2-204
 CALCulate:TDIagram:MARKer<x>:DELTA:X[:
 TIME]?, 2-206
 CALCulate:TDIagram:MARKer<x>:DELTA:
 Y?, 2-206
 CALCulate:TDIagram:MARKer<x>:
 MAXimum, 2-207
 CALCulate:TDIagram:MARKer<x>:PEAK:
 HIGHer, 2-208
 CALCulate:TDIagram:MARKer<x>:PEAK:
 LEFT, 2-208
 CALCulate:TDIagram:MARKer<x>:PEAK:
 LOWer, 2-209
 CALCulate:TDIagram:MARKer<x>:PEAK:
 RIGHT, 2-209
 CALCulate:TDIagram:MARKer<x>:X[:
 TIME], 2-210
 CALCulate:TDIagram:MARKer<x>:Y?, 2-210
 CALCulate:TOVerview:MARKer<x>:DELTA:
 X?, 2-211
 CALCulate:TOVerview:MARKer<x>:DELTA:
 Y?, 2-211
 CALCulate:TOVerview:MARKer<x>:
 MAXimum, 2-212
 CALCulate:TOVerview:MARKer<x>:PEAK:
 HIGHer, 2-212
 CALCulate:TOVerview:MARKer<x>:PEAK:
 LEFT, 2-213
 CALCulate:TOVerview:MARKer<x>:PEAK:
 LOWer, 2-213
 CALCulate:TOVerview:MARKer<x>:PEAK:
 RIGHT, 2-214
 CALCulate:TOVerview:MARKer<x>:X, 2-214
 CALCulate:TOVerview:MARKer<x>:Y?, 2-215
 CALibration:CORRection:EXTErnal:EDIT<x>:
 LABel, 2-216
 CALibration:CORRection:EXTErnal:EDIT<x>:
 NEW, 2-217
 CALibration:CORRection:EXTErnal:EDIT<x>:
 STATe, 2-217
 CALibration:CORRection:EXTErnal:GAIN:
 STATe, 2-218
 CALibration:CORRection:EXTErnal:GAIN[:
 MAGNitude], 2-218
 CALibration:CORRection:EXTErnal:PROBE:
 CONNect?, 2-219

CALibration:CORRection:EXTErnal:PROBE:
 STATe, 2-220
 CALibration:CORRection:EXTErnal:PROBE[:
 MAGNitude]?, 2-219
 CALibration:CORRection:EXTErnal:TYPE, 2-220
 CALibration:ABORt, 2-215
 CALibration:AUTO, 2-216
 *CLS, 2-221

D

DISPlay:{AM|FM|PM}:MARKer:SHOW:
 STATe, 2-228
 DISPlay:{AM|FM|PM}:WINDow:TRACe:
 GRATicule:GRID:STATe, 2-229
 DISPlay:{AM|FM|PM}:X:RSCale, 2-229
 DISPlay:{AM|FM|PM}:X[:SCALe]:AUTO, 2-230
 DISPlay:{AM|FM|PM}:X[:SCALe]:FULL, 2-230
 DISPlay:{AM|FM|PM}:X[:SCALe]:OFFSet, 2-230
 DISPlay:{AM|FM|PM}:Y:RSCale, 2-231
 DISPlay:{AM|FM|PM}:Y[:SCALe], 2-231
 DISPlay:{AM|FM|PM}:Y[:SCALe]:OFFSet, 2-232
 DISPlay:ACPower:MARKer:SHOW:STATe, 2-222
 DISPlay:ACPower:PLEVel:SHOW:STATe, 2-222
 DISPlay:ACPower:RESet:SCALe, 2-223
 DISPlay:ACPower:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-223
 DISPlay:ACPower:X[:SCALe], 2-224
 DISPlay:ACPower:X[:SCALe]:AUTO, 2-224
 DISPlay:ACPower:X[:SCALe]:OFFSet, 2-225
 DISPlay:ACPower:Y[:SCALe], 2-225
 DISPlay:ACPower:Y[:SCALe]:AUTO, 2-226
 DISPlay:ACPower:Y[:SCALe]:OFFSet, 2-226
 DISPlay:ADEMod:MEASview:DELeTe, 2-227
 DISPlay:ADEMod:MEASview:NEW, 2-227
 DISPlay:ADEMod:MEASview:SELeCt, 2-228
 DISPlay:AVTime:LEGend:STATe, 2-233
 DISPlay:AVTime:MARKer:SHOW:STATe, 2-233
 DISPlay:AVTime:RESet, 2-234
 DISPlay:AVTime:TRIGger:LEVel:STATe, 2-234
 DISPlay:AVTime:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-235
 DISPlay:AVTime:X:RSCale, 2-235
 DISPlay:AVTime:X[:SCALe]:AUTO, 2-236
 DISPlay:AVTime:X[:SCALe]:AUTO:STATe, 2-236
 DISPlay:AVTime:X[:SCALe]:FULL, 2-237
 DISPlay:AVTime:X[:SCALe]:MAXimum?, 2-237
 DISPlay:AVTime:X[:SCALe]:MINimum?, 2-238

- DISPlay:AVTime:X[:SCALE]:OFFSet, 2-238
DISPlay:AVTime:X[:SCALE]:OFFSet:
 MAXimum?, 2-239
DISPlay:AVTime:X[:SCALE]:OFFSet:
 MINimum?, 2-239
DISPlay:AVTime:Y:RSCale, 2-240
DISPlay:AVTime:Y[:SCALE]:FULL, 2-240
DISPlay:AVTime:Y[:SCALE]:OFFSet, 2-241
DISPlay:CCDF:LEGend:STATE, 2-241
DISPlay:CCDF:WINDow:TRACe:GRATICule:GRID:
 STATE, 2-242
DISPlay:CONSte:MPHase, 2-242
DISPlay:CONSte:WINDow:TRACe:GRATICule:
 GRID:STATE, 2-243
DISPlay:DDEMod:MEASview:DELeTe, 2-243
DISPlay:DDEMod:MEASview:NEW, 2-244
DISPlay:DDEMod:MEASview:SELeCt, 2-245
DISPlay:DDEMod:RADix, 2-245
DISPlay:DDEMod:X[:SCALE], 2-246
DISPlay:DDEMod:X[:SCALE]:AUTO, 2-247
DISPlay:DDEMod:X[:SCALE]:AUTO:STATE, 2-247
DISPlay:DDEMod:X[:SCALE]:MAXimum?, 2-248
DISPlay:DDEMod:X[:SCALE]:MINimum?, 2-248
DISPlay:DDEMod:X[:SCALE]:OFFSet, 2-249
DISPlay:DDEMod:X[:SCALE]:OFFSet:
 MAXimum?, 2-249
DISPlay:DDEMod:X[:SCALE]:OFFSet:
 MINimum?, 2-250
DISPlay:DDEMod:X[:SCALE]:RESet, 2-250
DISPlay:DIAGram:X[:SCALE], 2-251
DISPlay:DIAGram:X[:SCALE]:RESet, 2-251
DISPlay:DIQVtime:WINDow:TRACe:GRATICule:
 GRID:STATE, 2-252
DISPlay:DIQVtime:Y[:SCALE], 2-252
DISPlay:DIQVtime:Y[:SCALE]:AUTO, 2-253
DISPlay:DIQVtime:Y[:SCALE]:OFFSet, 2-253
DISPlay:DPSA:LEGend:STATE, 2-253
DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:
 STATE, 2-254
DISPlay:DPSA:Y[:SCALE]:PDIVision, 2-254
DISPlay:EDIagram:WINDow:TRACe:GRATICule:
 GRID:STATE, 2-255
DISPlay:EDIagram:Y[:SCALE], 2-255
DISPlay:EDIagram:Y[:SCALE]:AUTO, 2-256
DISPlay:EDIagram:Y[:SCALE]:OFFSet, 2-256
DISPlay:EVM:WINDow:TRACe:GRATICule:GRID:
 STATE, 2-257
DISPlay:EVM:Y[:SCALE], 2-257
DISPlay:EVM:Y[:SCALE]:AUTO, 2-258
DISPlay:EVM:Y[:SCALE]:OFFSet, 2-258
DISPlay:FDVTime:WINDow:TRACe:GRATICule:
 GRID:STATE, 2-259
DISPlay:FDVTime:Y[:SCALE], 2-259
DISPlay:FDVTime:Y[:SCALE]:AUTO, 2-260
DISPlay:FDVTime:Y[:SCALE]:OFFSet, 2-260
DISPlay:FVTime:WINDow:TRACe:GRATICule:
 GRID:STATE, 2-260
DISPlay:FVTime:X[:SCALE], 2-261
DISPlay:FVTime:X[:SCALE]:AUTO, 2-262
DISPlay:FVTime:X[:SCALE]:AUTO:STATE, 2-262
DISPlay:FVTime:X[:SCALE]:MAXimum?, 2-263
DISPlay:FVTime:X[:SCALE]:MINimum?, 2-263
DISPlay:FVTime:X[:SCALE]:OFFSet, 2-264
DISPlay:FVTime:X[:SCALE]:OFFSet:
 MAXimum?, 2-264
DISPlay:FVTime:X[:SCALE]:OFFSet:
 MINimum?, 2-265
DISPlay:FVTime:Y[:SCALE], 2-265
DISPlay:FVTime:Y[:SCALE]:AUTO, 2-266
DISPlay:FVTime:Y[:SCALE]:OFFSet, 2-266
DISPlay:GENeral:MEASview:DELeTe, 2-267
DISPlay:GENeral:MEASview:NEW, 2-268
DISPlay:GENeral:MEASview:SELeCt, 2-268
DISPlay:GPRF:MEASview:DELeTe, 2-269
DISPlay:GPRF:MEASview:NEW, 2-269
DISPlay:GPRF:MEASview:SELeCt, 2-270
DISPlay:IQVTime:WINDow:TRACe:GRATICule:
 GRID:STATE, 2-271
DISPlay:IQVTime:X[:SCALE], 2-271
DISPlay:IQVTime:X[:SCALE]:AUTO, 2-272
DISPlay:IQVTime:X[:SCALE]:AUTO:STATE, 2-272
DISPlay:IQVTime:X[:SCALE]:MAXimum?, 2-273
DISPlay:IQVTime:X[:SCALE]:MINimum?, 2-273
DISPlay:IQVTime:X[:SCALE]:OFFSet, 2-274
DISPlay:IQVTime:X[:SCALE]:OFFSet:
 MAXimum?, 2-275
DISPlay:IQVTime:X[:SCALE]:OFFSet:
 MINimum?, 2-275
DISPlay:IQVTime:Y[:SCALE], 2-276
DISPlay:IQVTime:Y[:SCALE]:AUTO, 2-276
DISPlay:IQVTime:Y[:SCALE]:OFFSet, 2-277
DISPlay:IQVTime:Y[:SCALE]:RESCale, 2-277
DISPlay:MCPower:MARKer:SHOW:STATE, 2-278
DISPlay:MCPower:PLEVel:SHOW:STATE, 2-278

DISPlay:MCPower:RESet:SCALe, 2-279
 DISPlay:MCPower:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-279
 DISPlay:MCPower:X[:SCALe], 2-280
 DISPlay:MCPower:X[:SCALe]:AUTO, 2-280
 DISPlay:MCPower:X[:SCALe]:OFFSet, 2-280
 DISPlay:MCPower:Y[:SCALe], 2-281
 DISPlay:MCPower:Y[:SCALe]:AUTO, 2-282
 DISPlay:MCPower:Y[:SCALe]:OFFSet, 2-282
 DISPlay:MERRor:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-283
 DISPlay:MERRor:Y[:SCALe], 2-283
 DISPlay:MERRor:Y[:SCALe]:AUTO, 2-284
 DISPlay:MERRor:Y[:SCALe]:OFFSet, 2-284
 DISPlay:OBWidth:MARKer:SHOW:STATe, 2-285
 DISPlay:OBWidth:RESet:SCALe, 2-285
 DISPlay:OBWidth:SELEcted:BANDwidth, 2-286
 DISPlay:OBWidth:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-286
 DISPlay:OBWidth:X[:SCALe], 2-287
 DISPlay:OBWidth:X[:SCALe]:AUTO, 2-287
 DISPlay:OBWidth:X[:SCALe]:OFFSet, 2-288
 DISPlay:OBWidth:Y[:SCALe], 2-288
 DISPlay:OBWidth:Y[:SCALe]:AUTO, 2-289
 DISPlay:OBWidth:Y[:SCALe]:OFFSet, 2-289
 DISPlay:PERRor:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-290
 DISPlay:PERRor:Y[:SCALe], 2-290
 DISPlay:PERRor:Y[:SCALe]:AUTO, 2-291
 DISPlay:PERRor:Y[:SCALe]:OFFSet, 2-291
 DISPlay:PHVTime:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-292
 DISPlay:PHVTime:X[:SCALe], 2-292
 DISPlay:PHVTime:X[:SCALe]:AUTO, 2-293
 DISPlay:PHVTime:X[:SCALe]:AUTO:STATe, 2-293
 DISPlay:PHVTime:X[:SCALe]:MAXimum?, 2-294
 DISPlay:PHVTime:X[:SCALe]:MINimum?, 2-294
 DISPlay:PHVTime:X[:SCALe]:OFFSet, 2-295
 DISPlay:PHVTime:X[:SCALe]:OFFSet:
 MAXimum?, 2-295
 DISPlay:PHVTime:X[:SCALe]:OFFSet:
 MINimum?, 2-296
 DISPlay:PHVTime:Y[:SCALe], 2-297
 DISPlay:PHVTime:Y[:SCALe]:AUTO, 2-297
 DISPlay:PHVTime:Y[:SCALe]:AXIS, 2-297
 DISPlay:PHVTime:Y[:SCALe]:AXIS:
 REFerence, 2-298
 DISPlay:PHVTime:Y[:SCALe]:OFFSet, 2-298
 DISPlay:PHVTime:Y[:SCALe]:RESCale, 2-299
 DISPlay:PNOise:LEGend:STATe, 2-299
 DISPlay:PNOise:MARKer:SHOW:STATe, 2-300
 DISPlay:PNOise:RESet:SCALe, 2-300
 DISPlay:PNOise:WINDow:TRACe:GRATicule:
 GRID:STATe, 2-301
 DISPlay:PNOise:X[:SCALe]:AUTO, 2-301
 DISPlay:PNOise:X[:SCALe]:START, 2-302
 DISPlay:PNOise:X[:SCALe]:STOP, 2-302
 DISPlay:PNOise:Y[:SCALe], 2-303
 DISPlay:PNOise:Y[:SCALe]:AUTO, 2-303
 DISPlay:PNOise:Y[:SCALe]:OFFSet, 2-304
 DISPlay:PNOise:Y[:SCALe]:PDIVision, 2-304
 DISPlay:PULSe:MEASview:DELeTe, 2-305
 DISPlay:PULSe:MEASview:NEW, 2-305
 DISPlay:PULSe:MEASview:SELEct, 2-306
 DISPlay:PULSe:RESult:ATX, 2-306
 DISPlay:PULSe:RESult:AVERAge, 2-307
 DISPlay:PULSe:RESult:DRODb, 2-307
 DISPlay:PULSe:RESult:DROOop, 2-308
 DISPlay:PULSe:RESult:DUTPct, 2-308
 DISPlay:PULSe:RESult:DUTRatio, 2-309
 DISPlay:PULSe:RESult:FALL, 2-309
 DISPlay:PULSe:RESult:FRDeviation, 2-310
 DISPlay:PULSe:RESult:IRAMplitude, 2-310
 DISPlay:PULSe:RESult:IRTime, 2-311
 DISPlay:PULSe:RESult:MFRReqerror, 2-311
 DISPlay:PULSe:RESult:MPHerror, 2-312
 DISPlay:PULSe:RESult:OVEDb, 2-312
 DISPlay:PULSe:RESult:OVERshoot, 2-313
 DISPlay:PULSe:RESult:PHDeviation, 2-313
 DISPlay:PULSe:RESult:PPFRequency, 2-314
 DISPlay:PULSe:RESult:PPower, 2-314
 DISPlay:PULSe:RESult:PPPHase, 2-315
 DISPlay:PULSe:RESult:RINTerval, 2-315
 DISPlay:PULSe:RESult:RIPDb, 2-316
 DISPlay:PULSe:RESult:RIPLe, 2-316
 DISPlay:PULSe:RESult:RISE, 2-317
 DISPlay:PULSe:RESult:RMSFreqerror, 2-317
 DISPlay:PULSe:RESult:RMSPherror, 2-318
 DISPlay:PULSe:RESult:RRATe, 2-318
 DISPlay:PULSe:RESult:TIME, 2-319
 DISPlay:PULSe:RESult:WIDTh, 2-319
 DISPlay:PULSe:SELEct:NUMBer, 2-320
 DISPlay:PULSe:SELEct:RESult, 2-320

- DISPlay:PULSe:STATistics:MARKer:SHOW:
 STATE, 2-321
 DISPlay:PULSe:STATistics:PLOT, 2-322
 DISPlay:PULSe:STATistics:WINDow:TRACe:
 GRATicule:GRID:STATE, 2-323
 DISPlay:PULSe:STATistics:X:RSCale, 2-323
 DISPlay:PULSe:STATistics:X[:SCALE]:
 NUMBer, 2-323
 DISPlay:PULSe:STATistics:X[:SCALE]:
 OFFSet, 2-324
 DISPlay:PULSe:STATistics:Y:RSCale, 2-325
 DISPlay:PULSe:STATistics:Y[:SCALE]:FULL, 2-325
 DISPlay:PULSe:STATistics:Y[:SCALE]:
 OFFSet, 2-326
 DISPlay:PULSe:STATistics:Y[:SCALE]:
 STOP?, 2-327
 DISPlay:PULSe:TRACe:MARKer:SHOW:
 STATE, 2-327
 DISPlay:PULSe:TRACe:POINt:SHOW, 2-328
 DISPlay:PULSe:TRACe:WINDow:TRACe:
 GRATicule:GRID:STATE, 2-328
 DISPlay:PULSe:TRACe:X:RSCale, 2-329
 DISPlay:PULSe:TRACe:X[:SCALE], 2-329
 DISPlay:PULSe:TRACe:X[:SCALE]:FULL, 2-330
 DISPlay:PULSe:TRACe:X[:SCALE]:OFFSet, 2-330
 DISPlay:PULSe:TRACe:X[:SCALE]:
 PDIVision, 2-331
 DISPlay:PULSe:TRACe:Y:RSCale, 2-331
 DISPlay:PULSe:TRACe:Y[:SCALE]:FULL, 2-332
 DISPlay:PULSe:TRACe:Y[:SCALE]:OFFSet, 2-332
 DISPlay:PULSe:TRACe:Y[:SCALE]:STOP?, 2-333
 DISPlay:SGRam:FREQuency:AUTO, 2-333
 DISPlay:SGRam:FREQuency:OFFSet, 2-334
 DISPlay:SGRam:FREQuency:SCALE, 2-334
 DISPlay:SGRam:TIME:AUTO, 2-335
 DISPlay:SGRam:TIME:OFFSet, 2-335
 DISPlay:SGRam:TIME:OVERlap, 2-336
 DISPlay:SGRam:TIME:SCALE, 2-336
 DISPlay:SPECTrum:FREQuency:AUTO, 2-337
 DISPlay:SPECTrum:FREQuency:OFFSet, 2-337
 DISPlay:SPECTrum:FREQuency[:SCALE], 2-338
 DISPlay:SPECTrum:MARKer:NOISe:MODE, 2-338
 DISPlay:SPECTrum:SCALE:LOG:STATE, 2-339
 DISPlay:SPECTrum:WINDow:TRACe:GRATicule:
 GRID:STATE, 2-339
 DISPlay:SPECTrum:WINDow:TRACe:LEGend:
 STATE, 2-340
 DISPlay:SPECTrum:X:LABel, 2-340
 DISPlay:SPECTrum:Y[:SCALE], 2-341
 DISPlay:SPECTrum:Y[:SCALE]:AUTO, 2-341
 DISPlay:SPECTrum:Y[:SCALE]:OFFSet, 2-342
 DISPlay:SPECTrum:Y[:SCALE]:PDIVision, 2-342
 DISPlay:SPECTrum:Y[:SCALE]:RESet, 2-343
 DISPlay:SPURious:MARKer:SHOW:STATE, 2-343
 DISPlay:SPURious:RESet:SCALE, 2-344
 DISPlay:SPURious:SCALE:LOG:STATE, 2-344
 DISPlay:SPURious:SELEct:NUMBer, 2-345
 DISPlay:SPURious:SHOW:LIMit, 2-345
 DISPlay:SPURious:WINDow:TRACe:GRATicule:
 GRID:STATE, 2-346
 DISPlay:SPURious:X[:SCALE]:AUTO, 2-346
 DISPlay:SPURious:X[:SCALE]:STARt, 2-347
 DISPlay:SPURious:X[:SCALE]:STOP, 2-347
 DISPlay:SPURious:Y[:SCALE], 2-348
 DISPlay:SPURious:Y[:SCALE]:AUTO, 2-348
 DISPlay:SPURious:Y[:SCALE]:OFFSet, 2-348
 DISPlay:TDIagram:WINDow:TRACe:GRATicule:
 GRID:STATE, 2-349
 DISPlay:TDIagram:Y[:SCALE], 2-349
 DISPlay:TDIagram:Y[:SCALE]:AUTO, 2-350
 DISPlay:TDIagram:Y[:SCALE]:OFFSet, 2-350
 DISPlay:TOVerview:WINDow:TRACe:GRATicule:
 GRID:STATE, 2-351
 DISPlay:TOVerview:X[:SCALE], 2-351
 DISPlay:TOVerview:X[:SCALE]:AUTO, 2-352
 DISPlay:TOVerview:X[:SCALE]:OFFSet, 2-352
 DISPlay:TOVerview:Y[:SCALE], 2-353
 DISPlay:TOVerview:Y[:SCALE]:AUTO, 2-353
 DISPlay:TOVerview:Y[:SCALE]:OFFSet, 2-354
 DISPlay:TOVerview:Y[:SCALE]:RESCale, 2-354
 DISPlay:WINDow:ACTive:MEASurement?, 2-355
 DISPlay:WINDow:COLor:SCHEme, 2-356
 DISPlay:WINDow:OPTimized:
 MEASurement?, 2-357
- E**
- *ESE, 2-358
 - *ESR?, 2-358
- F**
- FETCh: {FM|PM}:FERRor?, 2-386
 - FETCh:ACPower:CHANnel:POWER?, 2-360
 - FETCh:ACPower:SPECTrum?, 2-360

- FETCh:AM:AMNegative?, 2-362
 FETCh:AM:AMPositive?, 2-362
 FETCh:AVTime:
 {FIRSt|SECOnd|THIRd|FOURth}?, 2-364
 FETCh:AVTime:AVERAge?, 2-363
 FETCh:AVTime:MAXimum?, 2-365
 FETCh:AVTime:MAXLocation?, 2-365
 FETCh:AVTime:MINimum?, 2-366
 FETCh:AVTime:MINLocation?, 2-366
 FETCh:AVTime:RESult?, 2-367
 FETCh:CCDF: {FIRSt|SECOnd|THIRd} :X?, 2-369
 FETCh:CCDF: {FIRSt|SECOnd|THIRd} :XY?, 2-369
 FETCh:CCDF: {FIRSt|SECOnd|THIRd} [:Y]?, 2-370
 FETCh:CONStE:FERRor?, 2-371
 FETCh:CONStE:RESults?, 2-371
 FETCh:DDEMod:StABle?, 2-373
 FETCh:DDEMod:SYNCh:WORD:LENGth?, 2-373
 FETCh:DDEMod:SYNCh:WORD:POStion?, 2-374
 FETCh:DIQVtime:FERRor?, 2-374
 FETCh:DPSA:RESults:TRACe<x>?, 2-376
 FETCh:DPSA:TRACe:AVERAge?, 2-377
 FETCh:DPSA:TRACe:BITMap?, 2-377
 FETCh:DPSA:TRACe:MATH?, 2-378
 FETCh:DPSA:TRACe:MAXimum?, 2-379
 FETCh:DPSA:TRACe:MINimum?, 2-379
 FETCh:EDIagram:FDEVIation?, 2-380
 FETCh:EDIagram:FERRor?, 2-380
 FETCh:FDVTime:FERRor?, 2-385
 FETCh:FDVTime:TRACe?, 2-385
 FETCh:FVTime:MAXimum?, 2-390
 FETCh:FVTime:MAXLocation?, 2-390
 FETCh:FVTime:MINimum?, 2-391
 FETCh:FVTime:MINLocation?, 2-391
 FETCh:FVTime:RESult?, 2-392
 FETCh:IQVTime:MAXimum?, 2-393
 FETCh:IQVTime:MAXLocation?, 2-394
 FETCh:IQVTime:MINimum?, 2-394
 FETCh:IQVTime:MINLocation?, 2-395
 FETCh:IQVTime:RESult?, 2-396
 FETCh:MCPower:ADJacent:CHANnEls?, 2-397
 FETCh:MCPower:CHANnel:POWer?, 2-398
 FETCh:MCPower:MAIn:CHANnEls?, 2-398
 FETCh:MCPower:SPEctrum?, 2-399
 FETCh:MERRor:FERRor?, 2-399
 FETCh:MERRor:PINDEx?, 2-400
 FETCh:OBWidth:FREQuency:ERRor?, 2-402
 FETCh:OBWidth:OBWidth:BANDwidth?, 2-403
 FETCh:OBWidth:OBWidth:LEFT:
 FREQuency?, 2-403
 FETCh:OBWidth:OBWidth:LEFT:LEVel?, 2-404
 FETCh:OBWidth:OBWidth:POWer?, 2-404
 FETCh:OBWidth:OBWidth:RIGHT:
 FREQuency?, 2-405
 FETCh:OBWidth:OBWidth:RIGHT:LEVel?, 2-405
 FETCh:OBWidth:SPEctrum?, 2-406
 FETCh:OBWidth:XDBBANDwidth:
 BANDwidth?, 2-406
 FETCh:OBWidth:XDBBANDwidth:LEFT:
 FREQuency?, 2-407
 FETCh:OBWidth:XDBBANDwidth:LEFT:
 LEVel?, 2-407
 FETCh:OBWidth:XDBBANDwidth:POWer?, 2-408
 FETCh:OBWidth:XDBBANDwidth:RIGHT:
 FREQuency?, 2-408
 FETCh:OBWidth:XDBBANDwidth:RIGHT:
 LEVel?, 2-409
 FETCh:PERRor:FERRor?, 2-409
 FETCh:PERRor:PINDEx?, 2-410
 FETCh:PHVTime:MAXimum?, 2-413
 FETCh:PHVTime:MAXLocation?, 2-413
 FETCh:PHVTime:MINimum?, 2-414
 FETCh:PHVTime:MINLocation?, 2-414
 FETCh:PHVTime:RESult?, 2-415
 FETCh:PNOise:CARRier:FERRor?, 2-419
 FETCh:PNOise:CARRier:POWer?, 2-419
 FETCh:PNOise:JITTer?, 2-420
 FETCh:PNOise:RESidual:FM?, 2-420
 FETCh:PNOise:RMS:PNOise?, 2-421
 FETCh:PNOise:SPEctrum<x>:X?, 2-421
 FETCh:PNOise:SPEctrum<x>:XY?, 2-422
 FETCh:PNOise:SPEctrum<x>[:Y]?, 2-422
 FETCh:PULSe:STATistics:ATX?, 2-439
 FETCh:PULSe:STATistics:AVERAge?, 2-440
 FETCh:PULSe:STATistics:DRODb?, 2-440
 FETCh:PULSe:STATistics:DRooP?, 2-441
 FETCh:PULSe:STATistics:DUTPct?, 2-442
 FETCh:PULSe:STATistics:DUTRatio?, 2-442
 FETCh:PULSe:STATistics:FALL?, 2-443
 FETCh:PULSe:STATistics:FRDeviation?, 2-444
 FETCh:PULSe:STATistics:IRAMplitude?, 2-444
 FETCh:PULSe:STATistics:IRTime?, 2-445
 FETCh:PULSe:STATistics:MFRReqerror?, 2-445
 FETCh:PULSe:STATistics:MPHerror?, 2-446
 FETCh:PULSe:STATistics:OVEDb?, 2-447

- FETCh:PULSe:STATistics:OVERshoot?, 2-447
- FETCh:PULSe:STATistics:PHDeviation?, 2-448
- FETCh:PULSe:STATistics:PPFRequency?, 2-449
- FETCh:PULSe:STATistics:PPOWer?, 2-449
- FETCh:PULSe:STATistics:PPPHase?, 2-450
- FETCh:PULSe:STATistics:RINTerval?, 2-451
- FETCh:PULSe:STATistics:RIPDb?, 2-451
- FETCh:PULSe:STATistics:RIPPLE?, 2-452
- FETCh:PULSe:STATistics:RISE?, 2-453
- FETCh:PULSe:STATistics:RMSFreqerror?, 2-453
- FETCh:PULSe:STATistics:RMSPherror?, 2-454
- FETCh:PULSe:STATistics:RRATE?, 2-454
- FETCh:PULSe:STATistics:WIDTH?, 2-455
- FETCh:PULSe:STATistics:X?, 2-456
- FETCh:PULSe:STATistics:XY?, 2-456
- FETCh:PULSe:STATistics[:Y]?, 2-457
- FETCh:PULSe:TRACe:X?, 2-458
- FETCh:PULSe:TRACe:XY?, 2-459
- FETCh:PULSe:TRACe[:Y]?, 2-459
- FETCh:PULSe[:RESult]:ATX?, 2-423
- FETCh:PULSe[:RESult]:AVERAge?, 2-423
- FETCh:PULSe[:RESult]:DRODb?, 2-424
- FETCh:PULSe[:RESult]:DROop?, 2-425
- FETCh:PULSe[:RESult]:DUTPct?, 2-425
- FETCh:PULSe[:RESult]:DUTRatio?, 2-426
- FETCh:PULSe[:RESult]:FALL?, 2-426
- FETCh:PULSe[:RESult]:FRDeviation?, 2-427
- FETCh:PULSe[:RESult]:IRAMplitude?, 2-428
- FETCh:PULSe[:RESult]:IRTime?, 2-428
- FETCh:PULSe[:RESult]:MFRreqerror?, 2-429
- FETCh:PULSe[:RESult]:MPHerror?, 2-429
- FETCh:PULSe[:RESult]:OVEDb?, 2-430
- FETCh:PULSe[:RESult]:OVERshoot?, 2-431
- FETCh:PULSe[:RESult]:PHDeviation?, 2-431
- FETCh:PULSe[:RESult]:PPFRequency?, 2-432
- FETCh:PULSe[:RESult]:PPOWer?, 2-432
- FETCh:PULSe[:RESult]:PPPHase?, 2-433
- FETCh:PULSe[:RESult]:RINTerval?, 2-434
- FETCh:PULSe[:RESult]:RIPDb?, 2-434
- FETCh:PULSe[:RESult]:RIPPLE?, 2-435
- FETCh:PULSe[:RESult]:RISE?, 2-435
- FETCh:PULSe[:RESult]:RMSFreqerror?, 2-436
- FETCh:PULSe[:RESult]:RMSPherror?, 2-437
- FETCh:PULSe[:RESult]:RRATE?, 2-437
- FETCh:PULSe[:RESult]:TIME?, 2-438
- FETCh:PULSe[:RESult]:WIDTH?, 2-438
- FETCh:RFIN:IQ:HEADer?, 2-461
- FETCh:RFIN:IQ:SCALE?, 2-462
- FETCh:RFIN:RECORD:IDS?, 2-463
- FETCh:SPECTrum:TRACe<x>?, 2-464
- FETCh:SPURious:CARRier:POWer?, 2-465
- FETCh:SPURious:COUNT?, 2-465
- FETCh:SPURious:PASS?, 2-466
- FETCh:SPURious:SPECTrum:X?, 2-466
- FETCh:SPURious:SPECTrum:XY?, 2-467
- FETCh:SPURious:SPECTrum[:Y]?, 2-467
- FETCh:SPURious:SPUR<x>:AMPLitude:
ABSolute?, 2-468
- FETCh:SPURious:SPUR<x>:AMPLitude:
RELative?, 2-468
- FETCh:SPURious:SPUR<x>:FREQuency:
ABSolute?, 2-469
- FETCh:SPURious:SPUR<x>:FREQuency:
RELative?, 2-469
- FETCh:SPURious:SPUR<x>:LIMit:
ABSolute?, 2-470
- FETCh:SPURious:SPUR<x>:LIMit:RELative?, 2-470
- FETCh:SPURious:SPUR<x>:LIMit:
VIOLation?, 2-471
- FETCh:SPURious:SPUR<x>:RANGe?, 2-471
- FETCh:SQUality:FREQuency:DEViation:
TABLe?, 2-472
- FETCh:SQUality:FREQuency:DEViation?, 2-472
- FETCh:SQUality:FREQuency:ERRor?, 2-473
- FETCh:SQUality:GAIN:IMBalance?, 2-474
- FETCh:SQUality:ORIGIN:OFFSet?, 2-474
- FETCh:SQUality:PEAK:EVM:DB:OFFSet?, 2-476
- FETCh:SQUality:PEAK:EVM:DB?, 2-475
- FETCh:SQUality:PEAK:EVM:LOCation:
OFFSet?, 2-477
- FETCh:SQUality:PEAK:EVM:LOCation?, 2-476
- FETCh:SQUality:PEAK:EVM:OFFSet?, 2-477
- FETCh:SQUality:PEAK:EVM?, 2-475
- FETCh:SQUality:PEAK:FERRor?, 2-478
- FETCh:SQUality:PEAK:MERRor:DB?, 2-479
- FETCh:SQUality:PEAK:MERRor:LOCation?, 2-479
- FETCh:SQUality:PEAK:MERRor?, 2-478
- FETCh:SQUality:PEAK:PERRor:LOCation?, 2-480
- FETCh:SQUality:PEAK:PERRor?, 2-480
- FETCh:SQUality:QUADrature:ERRor?, 2-481
- FETCh:SQUality:RMS:EVM:DB:OFFSet?, 2-483
- FETCh:SQUality:RMS:EVM:DB?, 2-482
- FETCh:SQUality:RMS:EVM:OFFSet?, 2-483
- FETCh:SQUality:RMS:EVM?, 2-482

FETCh:SQUality:RMS:FERRor?, 2-484
 FETCh:SQUality:RMS:MER:DB?, 2-484
 FETCh:SQUality:RMS:MERRor:DB?, 2-485
 FETCh:SQUality:RMS:MERRor?, 2-485
 FETCh:SQUality:RMS:PERRor?, 2-486
 FETCh:SQUality:SYMBOL:LENGth?, 2-486
 FETCh:SQUality:SYMBOL:RATE:ERRor?, 2-487
 FETCh:SQUality:SYMBOL:RATE?, 2-486
 FETCh:TDIagram:FERRor?, 2-487
 FETCh:TDIagram:TRACe?, 2-488
 FETCh:{AM|FM|PM}?, 2-361
 FETCh:ACPower?, 2-359
 FETCh:AM:AMINdex?, 2-361
 FETCh:AM:RESult?, 2-363
 FETCh:CCDF?, 2-368
 FETCh:CONSte:TRACe?, 2-372
 FETCh:DIQVtime:I?, 2-375
 FETCh:DIQVtime:Q?, 2-375
 FETCh:EDIagram:I?, 2-381
 FETCh:EDIagram:Q?, 2-381
 FETCh:EVM:FERRor?, 2-382
 FETCh:EVM:PEAK?, 2-383
 FETCh:EVM:PINDEX?, 2-383
 FETCh:EVM:RMS?, 2-384
 FETCh:EVM:TRACe?, 2-384
 FETCh:FM:PHALf?, 2-386
 FETCh:FM:PNEGative?, 2-387
 FETCh:FM:PPOSitive?, 2-387
 FETCh:FM:PTPeak?, 2-388
 FETCh:FM:RESult?, 2-388
 FETCh:FM:RMS?, 2-389
 FETCh:FVTime?, 2-389
 FETCh:IQVTime:I?, 2-393
 FETCh:IQVTime:Q?, 2-396
 FETCh:MERRor:PEAK?, 2-400
 FETCh:MERRor:RMS?, 2-401
 FETCh:MERRor:TRACe?, 2-401
 FETCh:PERRor:PEAK?, 2-410
 FETCh:PERRor:RMS?, 2-411
 FETCh:PERRor:TRACe?, 2-411
 FETCh:PHVTime?, 2-412
 FETCh:PM:PNEGative?, 2-415
 FETCh:PM:PPOSitive?, 2-416
 FETCh:PM:PTPeak?, 2-416
 FETCh:PM:RESult?, 2-417
 FETCh:PM:RMS?, 2-417
 FETCh:PNOise:ALL?, 2-418

FETCh:RFIN:IQ?, 2-460
 FETCh:SGRam?, 2-463
 FETCh:SQUality:RHO?, 2-481
 FETCh:TOVerview?, 2-489

I

*IDN?, 2-489
 INITiate[:IMMediate], 2-490
 INITiate:CONTInuous, 2-490
 INPut: {MLEVel|RLEVel}, 2-493
 INPut:CORRection:EXTeRnal:EDIT<x>:
 INTeRpolation, 2-491
 INPut:CORRection:EXTeRnal:EDIT<x>:NEW, 2-492
 INPut:CORRection:EXTeRnal:TYPE, 2-492
 INPut[:RF]:ATTenuation, 2-493
 INPut[:RF]:ATTenuation:AUTO, 2-494
 INPut[:RF]:ATTenuation:MONitor:STATE, 2-494
 INPut[:RF]:GAIN:STATE, 2-495

M

MMEMory: {AM|FM|PM}:LOAD:TRACe, 2-495
 MMEMory: {AM|FM|PM}:SHOW:TRACe<x>, 2-496
 MMEMory: {AM|FM|PM}:STORE:TRACe, 2-496
 MMEMory:AVTime:LOAD:TRACe<x>, 2-497
 MMEMory:AVTime:SHOW:TRACe<x>, 2-497
 MMEMory:AVTime:STORE:TRACe<x>, 2-498
 MMEMory:CALibration:LOAD:CORRection:
 EXTeRnal:EDIT<x>, 2-498
 MMEMory:CALibration:STORE:CORRection:
 EXTeRnal:EDIT<x>, 2-499
 MMEMory:CCDF:LOAD:TRACe<x>, 2-499
 MMEMory:CCDF:SHOW:TRACe<x>, 2-500
 MMEMory:CCDF:STORE:TRACe<x>, 2-500
 MMEMory:DDEMod:LOAD:FILTer:MEASurement:
 UOTHer, 2-501
 MMEMory:DDEMod:LOAD:FILTer:MEASurement:
 USER<x>, 2-501
 MMEMory:DDEMod:LOAD:FILTer:REFeRence:
 UOTHer, 2-502
 MMEMory:DDEMod:LOAD:FILTer:REFeRence:
 USER<x>, 2-502
 MMEMory:DDEMod:LOAD:SYMBOL:MAP, 2-503
 MMEMory:DPSA:LOAD:TRACe<x>, 2-503
 MMEMory:DPSA:SHOW:TRACe<x>, 2-504
 MMEMory:DPSA:STORE:TRACe<x>, 2-504
 MMEMory:FVTime:LOAD:TRACe, 2-505

MMEMory:FVTIME:SHOW:TRACe<x>, 2-505
 MMEMory:FVTime:STORE:TRACe, 2-506
 MMEMory:IQVTime:LOAD:TRACe:I, 2-506
 MMEMory:IQVTime:LOAD:TRACe:Q, 2-506
 MMEMory:IQVTIME:SHOW:TRACe:I, 2-507
 MMEMory:IQVTIME:SHOW:TRACe<x>:Q, 2-507
 MMEMory:IQVTime:STORE:TRACe:I, 2-508
 MMEMory:IQVTime:STORE:TRACe:Q, 2-508
 MMEMory:PHVTime:LOAD:TRACe, 2-511
 MMEMory:PHVTime:SHOW:TRACe, 2-512
 MMEMory:PHVTime:STORE:TRACe, 2-512
 MMEMory:PNOise:LOAD:TRACe<x>, 2-513
 MMEMory:PNOise:SHOW:TRACe<x>, 2-513
 MMEMory:PNOise:STORE:TRACe<x>, 2-514
 MMEMory:SGRam:LOAD:TRACe, 2-514
 MMEMory:SGRam:SHOW:TRACe, 2-515
 MMEMory:SGRam:STORE:TRACe, 2-515
 MMEMory:SPECTrum:LOAD:TRACe, 2-516
 MMEMory:SPECTrum:SHOW:TRACe<x>, 2-516
 MMEMory:SPECTrum:STORE:TRACe<x>, 2-517
 MMEMory:SPURious:LOAD:TABLE, 2-517
 MMEMory:SPURious:STORE:TABLE, 2-518
 MMEMory:STORE:IQ:CSV, 2-519
 MMEMory:STORE:IQ:MAT, 2-519
 MMEMory:STORE:IQ:SELEct:FRAMES, 2-520
 MMEMory:STORE:IQ:SELEct:LENGth, 2-520
 MMEMory:STORE:MSTate, 2-520
 MMEMory:STORE:RESuLts, 2-521
 MMEMory:STORE:SCReen, 2-521
 MMEMory:TOVerview:LOAD:TRACe1, 2-523
 MMEMory:TOVerview:SHOW:TRACe1, 2-523
 MMEMory:TOVerview:STORE:TRACe1, 2-524
 MMEMory:LOAD:IQ, 2-509
 MMEMory:LOAD:STATe, 2-509
 MMEMory:LOAD:TRACe, 2-510
 MMEMory:STORE:IQ, 2-518
 MMEMory:STORE:STATe, 2-522
 MMEMory:STORE:TRACe, 2-522

O

*OPC, 2-525
 *OPT?, 2-525
 OUTPut:IF: {BANDwidth|BWIDTH}, 2-526
 OUTPut:NOISe[:STATe], 2-527
 OUTPut:IF[:STATe], 2-526
 OUTPut:IQ[:STATe], 2-527
 Overview of the Manual, 1-1

R

READ: {FM|PM}:FERRor?, 2-554
 READ:ACPower:CHANnel:POWER?, 2-529
 READ:ACPower:SPECTrum?, 2-529
 READ:AVTime:
 {FIRSt|SECond|THIRd|FOURth}?, 2-533
 READ:AVTime:AVERAge?, 2-532
 READ:AVTime:MAXimum?, 2-534
 READ:AVTime:MAXLocation?, 2-534
 READ:AVTime:MINimum?, 2-535
 READ:AVTime:MINLocation?, 2-535
 READ:CCDF: {FIRSt|SECond|THIRd}:X?, 2-537
 READ:CCDF: {FIRSt|SECond|THIRd}:XY?, 2-538
 READ:CCDF: {FIRSt|SECond|THIRd}[:Y]?, 2-539
 READ:CONSte:RESuLts?, 2-540
 READ:DIQVtime:FERRor?, 2-542
 READ:DPSA:RESuLts:TRACe<x>?, 2-544
 READ:DPSA:TRACe:AVERAge?, 2-545
 READ:DPSA:TRACe:BITMap?, 2-545
 READ:DPSA:TRACe:MATH?, 2-546
 READ:DPSA:TRACe:MAXimum?, 2-547
 READ:DPSA:TRACe:MINimum?, 2-547
 READ:EDIagram:FDEVIation?, 2-548
 READ:EDIagram:FERRor?, 2-548
 READ:FDVTime:FERRor?, 2-553
 READ:FVTime:MAXimum?, 2-558
 READ:FVTime:MAXLocation?, 2-558
 READ:FVTime:MINimum?, 2-559
 READ:FVTime:MINLocation?, 2-559
 READ:IQVTime:MAXimum?, 2-561
 READ:IQVTime:MAXLocation?, 2-562
 READ:IQVTime:MINimum?, 2-562
 READ:IQVTime:MINLocation?, 2-563
 READ:IQVTime:RESuLt?, 2-564
 READ:MCPower:ADJacent:CHANnels?, 2-564
 READ:MCPower:CHANnel:POWER?, 2-565
 READ:MCPower:MAIN:CHANnels?, 2-566
 READ:MCPower:SPECTrum?, 2-566
 READ:OBWidth:FREQuency:ERRor?, 2-570
 READ:OBWidth:OBWidth:BANDwidth?, 2-570
 READ:OBWidth:OBWidth:LEFT:
 FREQuency?, 2-571
 READ:OBWidth:OBWidth:LEFT:LEVel?, 2-571
 READ:OBWidth:OBWidth:POWER?, 2-572
 READ:OBWidth:OBWidth:RIGHT:
 FREQuency?, 2-572
 READ:OBWidth:OBWidth:RIGHT:LEVel?, 2-573

READ:OBWidth:SPECTrum?, 2-573
 READ:OBWidth:XDBBbandwidth:
 BANDwidth?, 2-574
 READ:OBWidth:XDBBbandwidth:LEFT:
 FREQuency?, 2-574
 READ:OBWidth:XDBBbandwidth:LEFT:
 LEVel?, 2-575
 READ:OBWidth:XDBBbandwidth:POWer?, 2-575
 READ:OBWidth:XDBBbandwidth:RIGHT:
 FREQuency?, 2-576
 READ:OBWidth:XDBBbandwidth:RIGHT:
 LEVel?, 2-576
 READ:PHVTime:MAXimum?, 2-580
 READ:PHVTime:MAXLocation?, 2-581
 READ:PHVTime:MINimum?, 2-581
 READ:PHVTime:MINLocation?, 2-582
 READ:PHVTime:RESult?, 2-582
 READ:PNOise:CARRier:FERRor?, 2-586
 READ:PNOise:CARRier:POWer?, 2-587
 READ:PNOise:RESidual:FM?, 2-588
 READ:PNOise:RMS:PNOise?, 2-588
 READ:PNOise:SPECTrum<x>:X?, 2-589
 READ:PNOise:SPECTrum<x>:XY?, 2-589
 READ:PNOise:SPECTrum<x>[:Y]?, 2-590
 READ:PULSe:STATistics:ATX?, 2-607
 READ:PULSe:STATistics:AVErAge?, 2-608
 READ:PULSe:STATistics:DRoDb?, 2-609
 READ:PULSe:STATistics:DRoOp?, 2-609
 READ:PULSe:STATistics:DUtPct?, 2-610
 READ:PULSe:STATistics:DUtRatio?, 2-611
 READ:PULSe:STATistics:FALL?, 2-611
 READ:PULSe:STATistics:FRDeviAtion?, 2-612
 READ:PULSe:STATistics:IRAMplitude?, 2-612
 READ:PULSe:STATistics:IRTime?, 2-613
 READ:PULSe:STATistics:MFReqerror?, 2-614
 READ:PULSe:STATistics:MPHerror?, 2-614
 READ:PULSe:STATistics:OVEDb?, 2-615
 READ:PULSe:STATistics:OVERshoot?, 2-616
 READ:PULSe:STATistics:PHDeviAtion?, 2-616
 READ:PULSe:STATistics:PPFRequency?, 2-617
 READ:PULSe:STATistics:PPOWer?, 2-617
 READ:PULSe:STATistics:PPPHasE?, 2-618
 READ:PULSe:STATistics:RINTerval?, 2-619
 READ:PULSe:STATistics:RIPDb?, 2-619
 READ:PULSe:STATistics:RIPple?, 2-620
 READ:PULSe:STATistics:RISE?, 2-621
 READ:PULSe:STATistics:RMSFRequerror?, 2-621
 READ:PULSe:STATistics:RMSPherror?, 2-622
 READ:PULSe:STATistics:RRATe?, 2-623
 READ:PULSe:STATistics:WIDTh?, 2-623
 READ:PULSe:STATistics:X?, 2-624
 READ:PULSe:STATistics:XY?, 2-625
 READ:PULSe:STATistics?, 2-606
 READ:PULSe:STATistics[:Y]?, 2-625
 READ:PULSe:TRACe:XY?, 2-627
 READ:PULSe:TRACe[:Y]?, 2-627
 READ:PULSe[:RESult]:ATX?, 2-590
 READ:PULSe[:RESult]:AVErAge?, 2-591
 READ:PULSe[:RESult]:DRoDb?, 2-592
 READ:PULSe[:RESult]:DRoOp?, 2-592
 READ:PULSe[:RESult]:DUtPct?, 2-593
 READ:PULSe[:RESult]:DUtRatio?, 2-594
 READ:PULSe[:RESult]:FALL?, 2-594
 READ:PULSe[:RESult]:FRDeviAtion?, 2-595
 READ:PULSe[:RESult]:IRAMplitude?, 2-595
 READ:PULSe[:RESult]:IRTime?, 2-596
 READ:PULSe[:RESult]:MFReqerror?, 2-596
 READ:PULSe[:RESult]:MPHerror?, 2-597
 READ:PULSe[:RESult]:OVEDb?, 2-598
 READ:PULSe[:RESult]:OVERshoot?, 2-598
 READ:PULSe[:RESult]:PHDeviAtion?, 2-599
 READ:PULSe[:RESult]:PPFRequency?, 2-599
 READ:PULSe[:RESult]:PPOWer?, 2-600
 READ:PULSe[:RESult]:PPPHasE?, 2-601
 READ:PULSe[:RESult]:RINTerval?, 2-601
 READ:PULSe[:RESult]:RIPDb?, 2-602
 READ:PULSe[:RESult]:RIPple?, 2-602
 READ:PULSe[:RESult]:RISE?, 2-603
 READ:PULSe[:RESult]:RMSFRequerror?, 2-604
 READ:PULSe[:RESult]:RMSPherror?, 2-604
 READ:PULSe[:RESult]:RRATe?, 2-605
 READ:PULSe[:RESult]:TIME?, 2-605
 READ:PULSe[:RESult]:WIDTh?, 2-606
 READ:SPECTrum:TRACe<x>?, 2-629
 READ:SPURious:CARRier:POWer?, 2-629
 READ:SPURious:COUNT?, 2-630
 READ:SPURious:SPECTrum:X?, 2-631
 READ:SPURious:SPECTrum:XY?, 2-631
 READ:SPURious:SPECTrum[:Y]?, 2-632
 READ:SPURious:SPUR<x>:AMPLitude:
 ABSolute?, 2-633
 READ:SPURious:SPUR<x>:AMPLitude:
 RELative?, 2-633

- READ:SPURious:SPUR<x>:FREQUency:
ABSolute?, 2-634
- READ:SPURious:SPUR<x>:FREQUency:
RELative?, 2-634
- READ:SPURious:SPUR<x>:LIMit:ABSolute?, 2-635
- READ:SPURious:SPUR<x>:LIMit:RELative?, 2-635
- READ:SPURious:SPUR<x>:LIMit:
VIOLation?, 2-636
- READ:SPURious:SPUR<x>:RANGe?, 2-636
- READ:SQUality:FREQUency:DEViation:
TABLe?, 2-637
- READ:SQUality:FREQUency:DEViation?, 2-637
- READ:SQUality:FREQUency:ERRor?, 2-638
- READ:SQUality:GAIN:IMBalance?, 2-639
- READ:SQUality:ORIGin:OFFSet?, 2-639
- READ:SQUality:PEAK:EVM:DB:OFFSet?, 2-641
- READ:SQUality:PEAK:EVM:DB?, 2-640
- READ:SQUality:PEAK:EVM:LOCation:
OFFSet?, 2-642
- READ:SQUality:PEAK:EVM:LOCation?, 2-641
- READ:SQUality:PEAK:EVM:OFFSet?, 2-642
- READ:SQUality:PEAK:EVM?, 2-640
- READ:SQUality:PEAK:FERRor?, 2-643
- READ:SQUality:PEAK:MERRor:DB?, 2-644
- READ:SQUality:PEAK:MERRor:LOCation?, 2-644
- READ:SQUality:PEAK:MERRor?, 2-643
- READ:SQUality:PEAK:PERRor:LOCation?, 2-645
- READ:SQUality:PEAK:PERRor?, 2-645
- READ:SQUality:QUADrature:ERRor?, 2-646
- READ:SQUality:RMS:EVM:DB:OFFSet?, 2-648
- READ:SQUality:RMS:EVM:DB?, 2-647
- READ:SQUality:RMS:EVM:OFFSet?, 2-648
- READ:SQUality:RMS:EVM?, 2-647
- READ:SQUality:RMS:FERRor?, 2-649
- READ:SQUality:RMS:MERRor:DB?, 2-649
- READ:SQUality:RMS:MERRor:DB?, 2-650
- READ:SQUality:RMS:MERRor?, 2-650
- READ:SQUality:RMS:PERRor?, 2-651
- READ:SQUality:SYMBol:LENGth?, 2-651
- READ:SQUality:SYMBol:RATE:ERRor?, 2-652
- READ:SQUality:SYMBol:RATE?, 2-651
- READ:TDIagram:FERRor?, 2-653
- READ:TDIagram:TRACe?, 2-653
- READ:{AM|FM|PM}?, 2-530
- READ:ACPower?, 2-528
- READ:AM:AMINdex?, 2-530
- READ:AM:AMNegative?, 2-531
- READ:AM:AMPositive?, 2-531
- READ:AM:RESult?, 2-532
- READ:AVTime:RESult?, 2-536
- READ:CCDF?, 2-537
- READ:CONSte:FERRor?, 2-540
- READ:CONSte:TRACe?, 2-541
- READ:DDEMod:STABle?, 2-542
- READ:DIQVtime:I?, 2-543
- READ:DIQVtime:Q?, 2-543
- READ:EDIagram:I?, 2-549
- READ:EDIagram:Q?, 2-549
- READ:EVM:FERRor?, 2-550
- READ:EVM:PEAK?, 2-550
- READ:EVM:PINDex?, 2-551
- READ:EVM:RMS?, 2-551
- READ:EVM:TRACe?, 2-552
- READ:FDVTime:TRACe?, 2-553
- READ:FM:PHALf?, 2-554
- READ:FM:PNEGative?, 2-555
- READ:FM:PPOSitive?, 2-555
- READ:FM:PTPeak?, 2-556
- READ:FM:RESult?, 2-556
- READ:FM:RMS?, 2-557
- READ:FVTime?, 2-557
- READ:FVTime:RESult?, 2-560
- READ:IQVTime:I?, 2-561
- READ:IQVTime:Q?, 2-563
- READ:MERRor:FERRor?, 2-567
- READ:MERRor:PEAK?, 2-568
- READ:MERRor:PINDex?, 2-568
- READ:MERRor:RMS?, 2-569
- READ:MERRor:TRACe?, 2-569
- READ:PERRor:FERRor?, 2-577
- READ:PERRor:PEAK?, 2-577
- READ:PERRor:PINDex?, 2-578
- READ:PERRor:RMS, 2-579
- READ:PERRor:TRACe?, 2-579
- READ:PHVTime?, 2-580
- READ:PM:PNEGative?, 2-583
- READ:PM:PPOSitive?, 2-583
- READ:PM:PTPeak?, 2-584
- READ:PM:RESult?, 2-584
- READ:PM:RMS?, 2-585
- READ:PNOise:ALL?, 2-585
- READ:PNOise:JITTer?, 2-587
- READ:PULSe:TRACe:X?, 2-626
- READ:SGRam?, 2-628

READ:SPURious:PASS?, 2-630
 READ:SQUality:RHO?, 2-646
 READ:TOVerview?, 2-654
 Related Documentation, v
 *RST, 2-654

S

[SENSe]:{AM|FM|PM}:{BANDwidth|BWIDth}:
 MEASurement, 2-670
 [SENSe]:{AM|FM|PM}:
 {MTPoints|MAXTracepoints}, 2-671
 [SENSe]:{AM|FM|PM}:CLEar:RESults, 2-670
 [SENSe]:{FM|PM}:BURSt:THReshold, 2-714
 [SENSe]:{FM|PM}:FREQuency:OFFSet, 2-714
 [SENSe]:{FM|PM}:FREQuency:OFFSet:
 MARKer, 2-715
 [SENSe]:{FM|PM}:FREQuency:SEARch:
 AUTO, 2-715
 [SENSe]:ACPower:{BANDwidth|BWIDth}:
 VIDEo, 2-658
 [SENSe]:ACPower:{BANDwidth|BWIDth}:VIDeo:
 STATe, 2-658
 [SENSe]:ACPower:{BANDwidth|BWIDth}[:
 RESolution], 2-656
 [SENSe]:ACPower:{BANDwidth|BWIDth}[:
 RESolution]:ACTual?, 2-657
 [SENSe]:ACPower:{BANDwidth|BWIDth}[:
 RESolution]:AUTO, 2-657
 [SENSe]:ACPower:AVERage, 2-655
 [SENSe]:ACPower:AVERage:COUNT, 2-656
 [SENSe]:ACPower:CHANnel:
 {BANDwidth|BWIDth}, 2-659
 [SENSe]:ACPower:CHANnel:FILTer, 2-659
 [SENSe]:ACPower:CHANnel:PAIRs, 2-660
 [SENSe]:ACPower:CHANnel:SPACing, 2-660
 [SENSe]:ACPower:CHIPrate, 2-661
 [SENSe]:ACPower:CLEar:RESults, 2-661
 [SENSe]:ACPower:FREQuency, 2-661
 [SENSe]:ACPower:FREQuency:STEP, 2-662
 [SENSe]:ACPower:FREQuency:STEP:AUTO, 2-662
 [SENSe]:ACPower:NFLoor:STATe, 2-663
 [SENSe]:ACPower:OPTimize:SPAN, 2-663
 [SENSe]:ACPower:POINTs:COUNT, 2-664
 [SENSe]:ACPower:RRCRolloff, 2-664
 [SENSe]:ACQuisition:{BANDwidth|BWIDth}, 2-665
 [SENSe]:ACQuisition:FFRame:ACTual?, 2-665
 [SENSe]:ACQuisition:FFRame:LIMit, 2-666
 [SENSe]:ACQuisition:FFRame:STATe, 2-666
 [SENSe]:ACQuisition:MEMory:AVAILable:
 SAMPLes?, 2-667
 [SENSe]:ACQuisition:MEMory:CAPacity[:
 TIME]?, 2-667
 [SENSe]:ACQuisition:MEMory:USED[:
 PERCent]?, 2-668
 [SENSe]:ACQuisition:MODE, 2-668
 [SENSe]:ACQuisition:SAMPLes, 2-669
 [SENSe]:ACQuisition:SEConds, 2-669
 [SENSe]:AM:DETECT:AMPLitude, 2-671
 [SENSe]:ANALysis:ADVanced:DITHer, 2-672
 [SENSe]:ANALysis:ADVanced:DITHer:HWARe:
 STATus?, 2-672
 [SENSe]:ANALysis:LENGth, 2-673
 [SENSe]:ANALysis:LENGth:ACTual?, 2-673
 [SENSe]:ANALysis:LENGth:AUTO, 2-674
 [SENSe]:ANALysis:REFeRence, 2-674
 [SENSe]:ANALysis:STARt, 2-675
 [SENSe]:ANALysis:STARt:AUTO, 2-675
 [SENSe]:AVTime:{BANDwidth|BWIDth}, 2-676
 [SENSe]:AVTime:{BANDwidth|BWIDth}:
 ACTual?, 2-676
 [SENSe]:AVTime:CLEar:RESults, 2-677
 [SENSe]:AVTime:MAXTracepoints, 2-677
 [SENSe]:AVTime:METHod, 2-678
 [SENSe]:CCDF:{BANDwidth|BWIDth}, 2-679
 [SENSe]:CCDF:TIME:TOTal:LENGth, 2-679
 [SENSe]:CCDF:TIME:TYPE, 2-680
 [SENSe]:DDEMod:{BANDwidth|BWIDth}:
 MODE, 2-683
 [SENSe]:DDEMod:{BANDwidth|BWIDth}:
 TINTerval, 2-683
 [SENSe]:DDEMod:{BANDwidth|BWIDth}:
 TINTerval:AUTO, 2-684
 [SENSe]:DDEMod:ANALysis:LENGth, 2-681
 [SENSe]:DDEMod:ANALysis:LENGth:
 ACTual?, 2-681
 [SENSe]:DDEMod:ANALysis:LENGth:
 AUTO, 2-682
 [SENSe]:DDEMod:BURSt:DETECT, 2-684
 [SENSe]:DDEMod:BURSt:THReshold, 2-685
 [SENSe]:DDEMod:CARRier:OFFSet, 2-686
 [SENSe]:DDEMod:CARRier:OFFSet:AUTO, 2-686
 [SENSe]:DDEMod:FILTer:ALPHa, 2-687
 [SENSe]:DDEMod:FILTer:MEASurement, 2-687
 [SENSe]:DDEMod:FILTer:REFeRence, 2-688

- [SENSe]:DDEMod:FREQuency:DEVIation, 2-689
- [SENSe]:DDEMod:FREQuency:DEVIation:
 AUTO, 2-690
- [SENSe]:DDEMod:MAGNitude:NORMalize, 2-690
- [SENSe]:DDEMod:MINDEX, 2-691
- [SENSe]:DDEMod:MINDEX:AUTO, 2-692
- [SENSe]:DDEMod:MODulation:TYPE, 2-692
- [SENSe]:DDEMod:PRESet, 2-693
- [SENSe]:DDEMod:SRATE, 2-696
- [SENSe]:DDEMod:SWAP:IQ, 2-696
- [SENSe]:DDEMod:SYMBOL:HSSHift, 2-696
- [SENSe]:DDEMod:SYMBOL:MAP:SOURce?, 2-697
- [SENSe]:DDEMod:SYMBOL:MAP[:STATe], 2-697
- [SENSe]:DDEMod:SYMBOL:PLOT:POSition, 2-698
- [SENSe]:DDEMod:SYMBOL:POINTs, 2-698
- [SENSe]:DDEMod:SYMBOL:RATE:SEARch, 2-699
- [SENSe]:DDEMod:SYNCh:WORD, 2-700
- [SENSe]:DDEMod:SYNCh:WORD:SYMBOL, 2-700
- [SENSe]:DDEMod:TIME:UNITs, 2-701
- [SENSe]:DPSA: {BANDwidth|BWIDth} :
 ACTual?, 2-704
- [SENSe]:DPSA: {BANDwidth|BWIDth} :
 OPTimization, 2-705
- [SENSe]:DPSA: {BANDwidth|BWIDth} [:
 RESolution]:AUTO, 2-705
- [SENSe]:DPSA:AUDio:DEMod:GAIN, 2-701
- [SENSe]:DPSA:AUDio:DEMod:RXBWidth, 2-702
- [SENSe]:DPSA:AUDio:DEMod:
 RXFREquency?, 2-702
- [SENSe]:DPSA:AUDio:DEMod:STATe, 2-703
- [SENSe]:DPSA:AUDio:DEMod:TUNE, 2-703
- [SENSe]:DPSA:AUDio:DEMod:TYPE, 2-704
- [SENSe]:DPSA:CLEar:RESults, 2-706
- [SENSe]:DPSA:COLor:MAXimum, 2-707
- [SENSe]:DPSA:COLor:MINimum, 2-708
- [SENSe]:DPSA:DDENsity:MEASurement:
 SHOW, 2-708
- [SENSe]:DPSA:DWELl:AUTO, 2-709
- [SENSe]:DPSA:FREQuency:CENTer, 2-710
- [SENSe]:DPSA:FREQuency:SPAN, 2-710
- [SENSe]:DPSA:FREQuency:SPAN:
 {BANDwidth|BWIDth} [:RESolution]:
 RATio, 2-711
- [SENSe]:DPSA:FREQuency:START, 2-711
- [SENSe]:DPSA:FREQuency:STEP, 2-712
- [SENSe]:DPSA:FREQuency:STEP:AUTO, 2-712
- [SENSe]:DPSA:FREQuency:STOP, 2-713
- [SENSe]:DPSA:POINTs:COUNT, 2-713
- [SENSe]:FVTime:CLEar:RESults, 2-716
- [SENSe]:FVTime:FREQuency:CENTer, 2-716
- [SENSe]:FVTime:FREQuency:SPAN, 2-717
- [SENSe]:FVTime:FREQuency:START, 2-717
- [SENSe]:FVTime:FREQuency:STEP, 2-718
- [SENSe]:FVTime:FREQuency:STEP:AUTO, 2-718
- [SENSe]:FVTime:FREQuency:STOP, 2-719
- [SENSe]:FVTime:MAXTracepoints, 2-720
- [SENSe]:IQVTime:CLEar:RESults, 2-720
- [SENSe]:IQVTime:FREQuency:CENTer, 2-721
- [SENSe]:IQVTime:FREQuency:SPAN, 2-721
- [SENSe]:IQVTime:FREQuency:START, 2-722
- [SENSe]:IQVTime:FREQuency:STEP, 2-722
- [SENSe]:IQVTime:FREQuency:STEP:AUTO, 2-723
- [SENSe]:IQVTime:FREQuency:STOP, 2-723
- [SENSe]:IQVTime:MAXTracepoints, 2-724
- [SENSe]:MCPower: {BANDwidth|BWIDth} :
 VIDeo, 2-727
- [SENSe]:MCPower: {BANDwidth|BWIDth} :VIDeo:
 STATe, 2-727
- [SENSe]:MCPower: {BANDwidth|BWIDth} [:
 RESolution], 2-725
- [SENSe]:MCPower: {BANDwidth|BWIDth} [:
 RESolution]:ACTual?, 2-726
- [SENSe]:MCPower: {BANDwidth|BWIDth} [:
 RESolution]:AUTO, 2-726
- [SENSe]:MCPower:AVERage, 2-724
- [SENSe]:MCPower:AVERage:COUNT, 2-725
- [SENSe]:MCPower:CHANnel:ADJacent:ADD, 2-728
- [SENSe]:MCPower:CHANnel:ADJacent:
 DELete, 2-728
- [SENSe]:MCPower:CHANnel:FILTer, 2-729
- [SENSe]:MCPower:CHANnel:MAIN:
 {BANDwidth|BWIDth}, 2-729
- [SENSe]:MCPower:CHANnel:MAIN:COUNT, 2-730
- [SENSe]:MCPower:CHANnel:MAIN:
 INACTive, 2-730
- [SENSe]:MCPower:CHANnel:MAIN:
 SPACing, 2-731
- [SENSe]:MCPower:CHIPrate, 2-731
- [SENSe]:MCPower:CLEar:RESults, 2-732
- [SENSe]:MCPower:FREQuency, 2-732
- [SENSe]:MCPower:FREQuency:STEP, 2-732
- [SENSe]:MCPower:FREQuency:STEP:AUTO, 2-733
- [SENSe]:MCPower:NFLoor:STATe, 2-733
- [SENSe]:MCPower:OPTimize:SPAN, 2-734

- [SENSe]:MCPower:POINts:COUNT, 2-734
- [SENSe]:MCPower:RCHannels:MAIN<x>, 2-735
- [SENSe]:MCPower:RCHannels:TOTal, 2-736
- [SENSe]:MCPower:RCHannels?, 2-735
- [SENSe]:MCPower:RRCRolloff, 2-736
- [SENSe]:MEASurement:FREQuency, 2-737
- [SENSe]:MEASurement:FREQuency:CENTer:
LOCK, 2-737
- [SENSe]:OBWidth: {BANDwidth|BWIDth} :
MEASurement, 2-739
- [SENSe]:OBWidth: {BANDwidth|BWIDth} :
VIDeo, 2-741
- [SENSe]:OBWidth: {BANDwidth|BWIDth} :VIDeo:
STATe, 2-741
- [SENSe]:OBWidth: {BANDwidth|BWIDth}[:
RESolution], 2-739
- [SENSe]:OBWidth: {BANDwidth|BWIDth}[:
RESolution]:ACTual?, 2-740
- [SENSe]:OBWidth: {BANDwidth|BWIDth}[:
RESolution]:AUTO, 2-740
- [SENSe]:OBWidth:AVERAge, 2-738
- [SENSe]:OBWidth:AVERAge:COUNT, 2-738
- [SENSe]:OBWidth:CLEar:RESults, 2-742
- [SENSe]:OBWidth:FREQuency:CENTer, 2-742
- [SENSe]:OBWidth:FREQuency:STEP, 2-742
- [SENSe]:OBWidth:FREQuency:STEP:AUTO, 2-743
- [SENSe]:OBWidth:PERCent, 2-743
- [SENSe]:OBWidth:XDBLevel, 2-744
- [SENSe]:PHVTime:CLEar:RESults, 2-744
- [SENSe]:PHVTime:FREQuency:CENTer, 2-745
- [SENSe]:PHVTime:FREQuency:SPAN, 2-745
- [SENSe]:PHVTime:FREQuency:START, 2-746
- [SENSe]:PHVTime:FREQuency:STEP, 2-746
- [SENSe]:PHVTime:FREQuency:STEP:AUTO, 2-747
- [SENSe]:PHVTime:FREQuency:STOP, 2-747
- [SENSe]:PHVTime:MAXTracepoints, 2-748
- [SENSe]:PM:PHASe:OFFSet, 2-749
- [SENSe]:PM:PHASe:OFFSet:MARKer, 2-749
- [SENSe]:PM:PHASe:SEARch:AUTO, 2-749
- [SENSe]:PNOise:AVERAge:COUNT, 2-750
- [SENSe]:PNOise:AVERAge:ENABLE, 2-750
- [SENSe]:PNOise:CARRier:FREQuency:
TRACk, 2-751
- [SENSe]:PNOise:CARRier:THReshold, 2-751
- [SENSe]:PNOise:CLEar:RESults, 2-752
- [SENSe]:PNOise:FREQuency:INTEgration:OFFSet:
START, 2-752
- [SENSe]:PNOise:FREQuency:INTEgration:OFFSet:
STOP, 2-753
- [SENSe]:PNOise:FREQuency:PLOT:OFFSet:
START, 2-753
- [SENSe]:PNOise:FREQuency:PLOT:OFFSet:
STOP, 2-754
- [SENSe]:PNOise:OPTimization, 2-754
- [SENSe]:PULSe:ANALyze:FDOMain:
MEASurement:TIME:ALENgtH, 2-756
- [SENSe]:PULSe:ANALyze:FDOMain:
MEASurement:TIME:METHod, 2-756
- [SENSe]:PULSe:ANALyze:FDOMain:
MEASurement:TIME:RLENgtH, 2-757
- [SENSe]:PULSe:ANALyze:FDOMain:
MEASurement:TIME:RLEVel, 2-757
- [SENSe]:PULSe:ANALyze:FDOMain:
MEASurement:TIME:START, 2-758
- [SENSe]:PULSe:ANALyze:IRESpOse:CORRection:
AMPLitude[:STATe], 2-758
- [SENSe]:PULSe:ANALyze:IRESpOse:
KOTime, 2-759
- [SENSe]:PULSe:ANALyze:IRESpOse:
MEASurement:TIME:ALENgtH, 2-759
- [SENSe]:PULSe:ANALyze:IRESpOse:
MEASurement:TIME:METHod, 2-760
- [SENSe]:PULSe:ANALyze:IRESpOse:
MEASurement:TIME:RLENgtH, 2-760
- [SENSe]:PULSe:ANALyze:IRESpOse:
MEASurement:TIME:RLEVel, 2-761
- [SENSe]:PULSe:ANALyze:IRESpOse:
MEASurement:TIME:START, 2-761
- [SENSe]:PULSe:ANALyze:LEVel, 2-762
- [SENSe]:PULSe:ANALyze:LEVel:FIFTy, 2-762
- [SENSe]:PULSe:ANALyze:LEVel:HUNDred, 2-763
- [SENSe]:PULSe:ANALyze:OVERshoot:
MEASurement:TIME:ALENgtH, 2-763
- [SENSe]:PULSe:ANALyze:OVERshoot:
MEASurement:TIME:METHod, 2-764
- [SENSe]:PULSe:ANALyze:OVERshoot:
MEASurement:TIME:RLENgtH, 2-764
- [SENSe]:PULSe:ANALyze:OVERshoot:
MEASurement:TIME:RLEVel, 2-765
- [SENSe]:PULSe:ANALyze:OVERshoot:
MEASurement:TIME:START, 2-765
- [SENSe]:PULSe:ANALyze:PMLOCation, 2-766
- [SENSe]:PULSe:ANALyze:POINt:LOCation, 2-766
- [SENSe]:PULSe:ANALyze:RFALl, 2-767

- [SENSe]:PULSe:ANALyze:RIPple, 2-767
- [SENSe]:PULSe:CARRier:FREQuency?, 2-768
- [SENSe]:PULSe:CARRier:OFFSet, 2-768
- [SENSe]:PULSe:CARRier:SEARCh, 2-769
- [SENSe]:PULSe:DETEct:MEASurement, 2-769
- [SENSe]:PULSe:DETEct:NUMBER, 2-770
- [SENSe]:PULSe:DETEct:POWER[:THReshold], 2-770
- [SENSe]:PULSe:DETEct:TIME[:THReshold], 2-771
- [SENSe]:PULSe:FILTer:
 - {BANDwidth|BWIDth}, 2-771
- [SENSe]:PULSe:FILTer:MEASurement, 2-772
- [SENSe]:PULSe:FREFerence:AUTO, 2-773
- [SENSe]:PULSe:FREFerence:CSLOpe, 2-773
- [SENSe]:PULSe:FREFerence:CSLOpe:AUTO, 2-774
- [SENSe]:PULSe:FREFerence:OFFSet, 2-774
- [SENSe]:PULSe:MODulation:TYPE, 2-775
- [SENSe]:PULSe:SIGNAL:TYPE, 2-775
- [SENSe]:PULSe:STATistics:HISTogram:
 - ORDinate, 2-776
- [SENSe]:PULSe:STATistics:HISTogram:
 - POINts, 2-776
- [SENSe]:PULSe:STATistics:HISTogram:POINts:
 - AUTO, 2-777
- [SENSe]:REANalyze:ACQuisition:SETTings?, 2-778
- [SENSe]:REANalyze:ALL, 2-778
- [SENSe]:REANalyze:CURREnt, 2-778
- [SENSe]:REANalyze:CURREnt:ACQuisition?, 2-779
- [SENSe]:REANalyze:CURREnt:FRAME?, 2-779
- [SENSe]:REANalyze:CURREnt:TIMestamp?, 2-779
- [SENSe]:REANalyze:DELEte:DATA, 2-780
- [SENSe]:REANalyze:FIRSt, 2-780
- [SENSe]:REANalyze:LAST, 2-780
- [SENSe]:REANalyze:NEXt, 2-780
- [SENSe]:REANalyze:PAUSE, 2-781
- [SENSe]:REANalyze:PREVious, 2-781
- [SENSe]:REANalyze:SELEct:ACQuisition:FIRSt:
 - TIMestamp?, 2-782
- [SENSe]:REANalyze:SELEct:ACQuisition:
 - FIRSt?, 2-781
- [SENSe]:REANalyze:SELEct:ACQuisition:LAST:
 - TIMestamp?, 2-782
- [SENSe]:REANalyze:SELEct:ACQuisition:
 - LAST?, 2-782
- [SENSe]:REANalyze:SELEct:ACQuisition:
 - START, 2-783
- [SENSe]:REANalyze:SELEct:ACQuisition:START:
 - TIMestamp?, 2-783
- [SENSe]:REANalyze:SELEct:ACQuisition:
 - STOP, 2-783
- [SENSe]:REANalyze:SELEct:ACQuisition:STOP:
 - TIMestamp?, 2-784
- [SENSe]:REANalyze:SELEct:ALL, 2-784
- [SENSe]:REANalyze:SELEct:FRAME:FIRSt:
 - TIMestamp?, 2-785
- [SENSe]:REANalyze:SELEct:FRAME:FIRSt?, 2-784
- [SENSe]:REANalyze:SELEct:FRAME:LAST:
 - TIMestamp?, 2-786
- [SENSe]:REANalyze:SELEct:FRAME:LAST?, 2-785
- [SENSe]:REANalyze:SELEct:FRAME:START, 2-786
- [SENSe]:REANalyze:SELEct:FRAME:START:
 - TIMestamp?, 2-786
- [SENSe]:REANalyze:SELEct:FRAME:STOP, 2-787
- [SENSe]:REANalyze:SELEct:FRAME:STOP:
 - TIMestamp?, 2-787
- [SENSe]:REANalyze:SPEed, 2-787
- [SENSe]:REANalyze:STOP, 2-788
- [SENSe]:REANalyze:TIMestamp:DECimal, 2-788
- [SENSe]:ROSCillator:SOURce, 2-788
- [SENSe]:SGRam: {BANDwidth|BWIDth} :
 - OPTimization, 2-789
- [SENSe]:SGRam: {BANDwidth|BWIDth} :
 - RESolution, 2-790
- [SENSe]:SGRam: {BANDwidth|BWIDth} :
 - VIDeo, 2-792
- [SENSe]:SGRam: {BANDwidth|BWIDth} :VIDeo:
 - STATe, 2-792
- [SENSe]:SGRam: {BANDwidth|BWIDth} [:
 - RESolution]:ACTual?, 2-790
- [SENSe]:SGRam: {BANDwidth|BWIDth} [:
 - RESolution]:AUTO, 2-791
- [SENSe]:SGRam: {BANDwidth|BWIDth} [:
 - RESolution]:MODE, 2-791
- [SENSe]:SGRam:COLor:MAXimum, 2-793
- [SENSe]:SGRam:COLor:MINimum, 2-794
- [SENSe]:SGRam:FFT:WINDow, 2-795
- [SENSe]:SGRam:FILTer[:SHAPE], 2-795
- [SENSe]:SGRam:FREQuency:CENTer, 2-796
- [SENSe]:SGRam:FREQuency:SPAN, 2-796
- [SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:
 - RESolution]:RATio, 2-797
- [SENSe]:SGRam:FREQuency:SPAN:
 - MAXimum, 2-797
- [SENSe]:SGRam:FREQuency:START, 2-798
- [SENSe]:SGRam:FREQuency:STEP, 2-798

- [SENSe]:SGRam:FREQuency:STEP:AUTO, 2-799
- [SENSe]:SGRam:FREQuency:STOP, 2-799
- [SENSe]:SPECtrum: {BANDwidth|BWIDth}:
OPTImization, 2-800
- [SENSe]:SPECtrum: {BANDwidth|BWIDth}:
VIDeo, 2-803
- [SENSe]:SPECtrum: {BANDwidth|BWIDth}:VIDeo:
STATe, 2-803
- [SENSe]:SPECtrum: {BANDwidth|BWIDth}[:
RESolution], 2-801
- [SENSe]:SPECtrum: {BANDwidth|BWIDth}[:
RESolution]:ACTual?, 2-801
- [SENSe]:SPECtrum: {BANDwidth|BWIDth}[:
RESolution]:AUTO, 2-802
- [SENSe]:SPECtrum: {BANDwidth|BWIDth}[:
RESolution]:MODE, 2-802
- [SENSe]:SPECtrum:CLEar:RESults, 2-804
- [SENSe]:SPECtrum:FFT:WINDow, 2-804
- [SENSe]:SPECtrum:FILTer[:SHAPE], 2-805
- [SENSe]:SPECtrum:FREQuency:CENTer, 2-805
- [SENSe]:SPECtrum:FREQuency:SPAN, 2-806
- [SENSe]:SPECtrum:FREQuency:SPAN:
BANDwidth[:RESolution]:RATio, 2-806
- [SENSe]:SPECtrum:FREQuency:STARt, 2-807
- [SENSe]:SPECtrum:FREQuency:STEP, 2-807
- [SENSe]:SPECtrum:FREQuency:STEP:AUTO, 2-808
- [SENSe]:SPECtrum:FREQuency:STOP, 2-808
- [SENSe]:SPECtrum:LENGth, 2-809
- [SENSe]:SPECtrum:LENGth:ACTual?, 2-810
- [SENSe]:SPECtrum:LENGth:AUTO, 2-810
- [SENSe]:SPECtrum:MAX:SPAN, 2-811
- [SENSe]:SPECtrum:POINts:COUNT, 2-811
- [SENSe]:SPECtrum:STARt, 2-812
- [SENSe]:SPECtrum:TIME:MODE, 2-812
- [SENSe]:SPURious:CARRier:
{BANDwidth|BWIDth}, 2-813
- [SENSe]:SPURious:CARRier:
{BANDwidth|BWIDth}:INTegration, 2-813
- [SENSe]:SPURious:CARRier:
{BANDwidth|BWIDth}[:RESolution], 2-814
- [SENSe]:SPURious:CARRier:
{BANDwidth|BWIDth}[:RESolution]:
AUTO, 2-814
- [SENSe]:SPURious:CARRier:DETection, 2-815
- [SENSe]:SPURious:CARRier:FREQuency, 2-815
- [SENSe]:SPURious:CARRier:THREshold, 2-816
- [SENSe]:SPURious:CLEar:RESults, 2-816
- [SENSe]:SPURious:LIST, 2-817
- [SENSe]:SPURious:MODE, 2-818
- [SENSe]:SPURious:OPTImization, 2-818
- [SENSe]:SPURious:POINts:COUNT, 2-819
- [SENSe]:SPURious:RANGe<x>:BANDwidth:
VIDeo, 2-819
- [SENSe]:SPURious:RANGe<x>:BANDwidth:
VIDeo:STATe, 2-820
- [SENSe]:SPURious:RANGe<x>:DETection, 2-821
- [SENSe]:SPURious:RANGe<x>:EXCURsion, 2-821
- [SENSe]:SPURious:RANGe<x>:FILTer[:
SHAPE], 2-822
- [SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]:
BANDwidth, 2-822
- [SENSe]:SPURious:RANGe<x>:FILTer[:SHAPE]:
BANDwidth:AUTO, 2-823
- [SENSe]:SPURious:RANGe<x>:FREQuency:
STARt, 2-823
- [SENSe]:SPURious:RANGe<x>:FREQuency:
STOP, 2-824
- [SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:
STARt, 2-825
- [SENSe]:SPURious:RANGe<x>:LIMit:ABSolute:
STOP, 2-825
- [SENSe]:SPURious:RANGe<x>:LIMit:MASK, 2-826
- [SENSe]:SPURious:RANGe<x>:LIMit:RELative:
STARt, 2-827
- [SENSe]:SPURious:RANGe<x>:LIMit:RELative:
STOP, 2-827
- [SENSe]:SPURious:RANGe<x>:STATe, 2-828
- [SENSe]:SPURious:RANGe<x>:THREshold, 2-828
- [SENSe]:SPURious:REFerence, 2-829
- [SENSe]:SPURious:REFerence:MANual:
POWEr, 2-829
- [SENSe]:SPURious[:FREQuency]:OVERlap?, 2-817
- [SENSe]:TOVerview:FREQuency:CENTer, 2-830
- [SENSe]:TOVerview:MAXTracepoints, 2-830
- [SENSe]:AVTime:SPAN, 2-678
- [SENSe]:CCDF:CLEar, 2-679
- [SENSe]:DPSA:COLor, 2-706
- [SENSe]:DPSA:DWELl, 2-709
- [SENSe]:POWEr:UNITs, 2-755
- [SENSe]:REANalyze, 2-777
- [SENSe]:SGRam:COLor, 2-793
- [SENSe]:USETtings, 2-831
- *SRE, 2-831
- STATus: {AM|FM|PM}:EVENTs?, 2-833

STATus:ACPower:EVENTs?, 2-832
 STATus:AVTime:EVENTs?, 2-833
 STATus:CONStE:EVENTs?, 2-834
 STATus:DIQVtime:EVENTs?, 2-835
 STATus:EDIagram:EVENTs?, 2-836
 STATus:FDVTime:EVENTs?, 2-838
 STATus:FVTime:EVENTs?, 2-838
 STATus:IQVTime:EVENTs?, 2-839
 STATus:MCPower:EVENTs?, 2-840
 STATus:MERRor:EVENTs?, 2-840
 STATus:OBWidth:EVENTs?, 2-841
 STATus:OPERation:CONDition?, 2-842
 STATus:OPERation:ENABle, 2-842
 STATus:OPERation:NTRansition, 2-843
 STATus:OPERation:PTRansition, 2-844
 STATus:OPERation[:EVENT]?, 2-843
 STATus:PERRor:EVENTs?, 2-844
 STATus:PHVTime:EVENTs?, 2-845
 STATus:PNOise:EVENTs?, 2-846
 STATus:PULSe:RESult:EVENTs?, 2-847
 STATus:PULSe:STATistics:EVENTs?, 2-847
 STATus:PULSe:TRACe:EVENTs?, 2-848
 STATus:QUEStionable:CALibration:
 CONDition?, 2-849
 STATus:QUEStionable:CALibration:ENABle, 2-849
 STATus:QUEStionable:CALibration:
 NTRansition, 2-850
 STATus:QUEStionable:CALibration:
 PTRansition, 2-851
 STATus:QUEStionable:CALibration[:EVENT]?, 2-850
 STATus:QUEStionable:CONDition?, 2-851
 STATus:QUEStionable:ENABle, 2-852
 STATus:QUEStionable:FREQuency:
 CONDition?, 2-853
 STATus:QUEStionable:FREQuency:ENABle, 2-854
 STATus:QUEStionable:FREQuency:
 NTRansition, 2-855
 STATus:QUEStionable:FREQuency:
 PTRansition, 2-855
 STATus:QUEStionable:FREQuency[:EVENT]?, 2-854
 STATus:QUEStionable:NTRansition, 2-856
 STATus:QUEStionable:PTRansition, 2-856
 STATus:QUEStionable[:EVENT]?, 2-853
 STATus:SGRAM:EVENTs?, 2-857
 STATus:SPECTrum:EVENTs?, 2-858
 STATus:SPURious:EVENTs?, 2-858
 STATus:SQUALity:EVENTs?, 2-859

STATus:TDIagram:EVENTs?, 2-860
 STATus:CCDF:EVENTs?, 2-834
 STATus:DPsA:EVENTs?, 2-836
 STATus:EVM:EVENTs?, 2-837
 STATus:PRESet, 2-846
 *STB?, 2-860
 SYSTem:COMMunicate:GPIB[:SELF]:
 ADDRess, 2-861
 SYSTem:ERRor:CODE:ALL?, 2-863
 SYSTem:ERRor:CODE[:NEXT]?, 2-863
 SYSTem:ERRor[:NEXT]?, 2-864
 SYSTem:DATE, 2-861
 SYSTem:ERRor:ALL?, 2-862
 SYSTem:ERRor:COUNt?, 2-864
 SYSTem:OPTions?, 2-865
 SYSTem:PRESet, 2-865
 SYSTem:TIME, 2-866
 SYSTem:VERSion?, 2-866

T

TRACe:{AM|FM|PM}:DETEction, 2-867
 TRACe:{AM|FM|PM}:FREeze, 2-868
 TRACe:{AM|FM|PM}:FUNction, 2-868
 TRACe:DIQVtime:ENABle:I, 2-869
 TRACe:DIQVtime:ENABle:Q, 2-870
 TRACe:DIQVtime:SELEct:I, 2-870
 TRACe:DIQVtime:SELEct:Q, 2-871
 TRACe:EDIagram:ENABle:I, 2-871
 TRACe:EDIagram:ENABle:Q, 2-872
 TRACe:EDIagram:SELEct:I, 2-872
 TRACe:EDIagram:SELEct:Q, 2-873
 TRACe:FVTime:AVERage:COUNt, 2-874
 TRACe:FVTime:COUNt:ENABle, 2-875
 TRACe:FVTime:COUNt:RESet, 2-875
 TRACe:FVTime:FUNction, 2-876
 TRACe:IQVTime:AVERage:COUNt, 2-877
 TRACe:IQVTime:COUNt:ENABle, 2-878
 TRACe:IQVTime:COUNt:RESet, 2-878
 TRACe:IQVTime:DETEction, 2-879
 TRACe:IQVTime:ENABle:I, 2-879
 TRACe:IQVTime:ENABle:Q, 2-880
 TRACe:IQVTime:FREeze, 2-880
 TRACe:IQVTime:FUNction, 2-881
 TRACe:IQVTime:SELEct:I, 2-881
 TRACe:IQVTime:SELEct:Q, 2-882
 TRACe:PHVTime:AVERage:COUNt, 2-883
 TRACe:PHVTime:COUNt:ENABle, 2-884

- TRACe:PHVTime:COUNT:RESet, 2-885
 TRACe:PHVTime:FREeze, 2-885
 TRACe:PHVTime:FUNcTION, 2-886
 TRACe:SGRam:DETEction, 2-886
 TRACe:SGRam:FUNcTION, 2-888
 TRACe:SGRam:FUNcTION:TIME, 2-888
 TRACe:SGRam:SELEct:LINE, 2-889
 TRACe:SPURious:COUNT, 2-889
 TRACe:SPURious:COUNT:ENABle, 2-890
 TRACe:SPURious:COUNT:RESet, 2-890
 TRACe:SPURious:FREeze, 2-891
 TRACe:SPURious:FUNcTION, 2-891
 TRACe: {AM|FM|PM}, 2-867
 TRACe:CONStE:MODE, 2-869
 TRACe:FVTime, 2-873
 TRACe:FVTime:COUNT, 2-874
 TRACe:FVTime:FREeze, 2-876
 TRACe:IQVTime:COUNT, 2-877
 TRACe:OBW:MAXHold, 2-882
 TRACe:PHVTime, 2-883
 TRACe:PHVTime:COUNT, 2-884
 TRACe:SGRam:FREeze, 2-887
 TRACe<x>:AVTime:AVERAge:COUNT, 2-896
 TRACe<x>:AVTime:AVERAge:RESet, 2-896
 TRACe<x>:AVTime:COUNT, 2-897
 TRACe<x>:AVTime:COUNT:ENABle, 2-898
 TRACe<x>:AVTime:COUNT:RESet, 2-898
 TRACe<x>:AVTime:DETEction, 2-899
 TRACe<x>:AVTime:FREeze, 2-899
 TRACe<x>:AVTime:FUNcTION, 2-900
 TRACe<x>:AVTime:LEFToperand, 2-900
 TRACe<x>:AVTime:RIGHToperand, 2-901
 TRACe<x>:AVTime:SELEct, 2-902
 TRACe<x>:CCDF:FREeze, 2-902
 TRACe<x>:CCDF:SELEct, 2-903
 TRACe<x>:CCDF:SHOW, 2-903
 TRACe<x>:DPSA:AVERAge:COUNT, 2-906
 TRACe<x>:DPSA:COLor:CURVe, 2-906
 TRACe<x>:DPSA:COLor:INTensity, 2-907
 TRACe<x>:DPSA:COLor:SCALE:AUTO, 2-907
 TRACe<x>:DPSA:DETEction, 2-908
 TRACe<x>:DPSA:DOT:PERsistent, 2-908
 TRACe<x>:DPSA:DOT:PERsistent:TYPE, 2-909
 TRACe<x>:DPSA:DOT:PERsistent:VARiable, 2-909
 TRACe<x>:DPSA:FREeze, 2-910
 TRACe<x>:DPSA:FUNcTION, 2-910
 TRACe<x>:DPSA:LEFToperand, 2-911
 TRACe<x>:DPSA:RIGHToperand, 2-912
 TRACe<x>:DPSA:SELEct, 2-912
 TRACe<x>:FVTime:DETEction, 2-913
 TRACe<x>:PHVTime:DETEction, 2-913
 TRACe<x>:PNOise:SELEct, 2-914
 TRACe<x>:PNOise:SHOW, 2-915
 TRACe<x>:PNOise:SMOothing:COUNT, 2-915
 TRACe<x>:PNOise:SMOothing:ENABle, 2-916
 TRACe<x>:PNOise:SMOothing:RESet, 2-916
 TRACe<x>:SPEcTrum, 2-917
 TRACe<x>:SPEcTrum:AVERAge:COUNT, 2-917
 TRACe<x>:SPEcTrum:AVERAge:RESet, 2-918
 TRACe<x>:SPEcTrum:COUNT, 2-918
 TRACe<x>:SPEcTrum:COUNT:ENABle, 2-919
 TRACe<x>:SPEcTrum:COUNT:RESet, 2-919
 TRACe<x>:SPEcTrum:DETEction, 2-920
 TRACe<x>:SPEcTrum:FREeze, 2-921
 TRACe<x>:SPEcTrum:FUNcTION, 2-921
 TRACe<x>:SPEcTrum:LEFToperand, 2-922
 TRACe<x>:SPEcTrum:RIGHToperand, 2-922
 TRACe<x>:SPEcTrum:SELEct, 2-923
 TRACe<x>:AVTime, 2-895
 TRACe<x>:CCDF:X, 2-904
 TRACe<x>:CCDF:Y?, 2-904
 TRACe<x>:DPSA, 2-905
 TRACe1:TOVerview:AVERAge:COUNT, 2-892
 TRACe1:TOVerview:COUNT, 2-893
 TRACe1:TOVerview:COUNT:ENABle, 2-893
 TRACe1:TOVerview:COUNT:RESet, 2-893
 TRACe1:TOVerview:DETEction, 2-894
 TRACe1:TOVerview:FREeze, 2-894
 TRACe1:TOVerview:FUNcTION, 2-895
 TRACe1:TOVerview, 2-892
 *TRG, 2-924
 TRIGger:DPSA:SHOW:FRAMES, 2-924
 TRIGger:MASK:NEW:AUTO, 2-926
 TRIGger[:SEQuence]:ADVanced:HOLDoff, 2-928
 TRIGger[:SEQuence]:ADVanced:HOLDoff:
 ENABle, 2-929
 TRIGger[:SEQuence]:ADVanced:SWEEP:
 MODE, 2-929
 TRIGger[:SEQuence]:ADVanced:SWEEP:SEGMENT:
 ENABle, 2-930
 TRIGger[:SEQuence]:EVENT:EXTFront:
 IMPedance, 2-930
 TRIGger[:SEQuence]:EVENT:EXTFront:
 LEVel, 2-931

- TRIGger[:SEquence]:EVENT:EXTFront:
SLOPe, 2-931
- TRIGger[:SEquence]:EVENT:EXTRear:
SLOPe, 2-931
- TRIGger[:SEquence]:EVENT:GATed, 2-932
- TRIGger[:SEquence]:EVENT:INPut:DDENsity:
AMPLitude, 2-932
- TRIGger[:SEquence]:EVENT:INPut:DDENsity:
AMPLitude:TOLerance, 2-933
- TRIGger[:SEquence]:EVENT:INPut:DDENsity:
FREQuency, 2-934
- TRIGger[:SEquence]:EVENT:INPut:DDENsity:
FREQuency:TOLerance, 2-934
- TRIGger[:SEquence]:EVENT:INPut:DDENsity:
THReshold, 2-935
- TRIGger[:SEquence]:EVENT:INPut:DDENsity:
VIOLation, 2-935
- TRIGger[:SEquence]:EVENT:INPut:FMASk:
{BANDwidth|BWIDth}{:RESolution}, 2-936
- TRIGger[:SEquence]:EVENT:INPut:FMASk:
BANDwidth|BWIDth[:RESolution]:
ACTual?, 2-937
- TRIGger[:SEquence]:EVENT:INPut:FMASk:
BANDwidth|BWIDth[:RESolution]:AUTO, 2-937
- TRIGger[:SEquence]:EVENT:INPut:FMASk:
VIOLation, 2-938
- TRIGger[:SEquence]:EVENT:INPut:LEVel, 2-939
- TRIGger[:SEquence]:EVENT:INPut:RUNT:
PULSe, 2-939
- TRIGger[:SEquence]:EVENT:INPut:RUNT:PULSe:
HIGH:LEVel, 2-940
- TRIGger[:SEquence]:EVENT:INPut:RUNT:PULSe:
LOW:LEVel, 2-940
- TRIGger[:SEquence]:EVENT:INPut:SLOPe, 2-941
- TRIGger[:SEquence]:EVENT:INPut:
TDBWidth, 2-941
- TRIGger[:SEquence]:EVENT:INPut:TDBWidth:
ACTual?, 2-942
- TRIGger[:SEquence]:EVENT:INPut:TDBWidth:
STATe, 2-942
- TRIGger[:SEquence]:EVENT:INPut:TYPE, 2-943
- TRIGger[:SEquence]:EVENT:SOURce, 2-943
- TRIGger[:SEquence]:FORCed, 2-944
- TRIGger[:SEquence]:IMMediate, 2-944
- TRIGger[:SEquence]:STATus, 2-945
- TRIGger[:SEquence]:TIME:DELay, 2-945
- TRIGger[:SEquence]:TIME:POSition, 2-946
- TRIGger[:SEquence]:TIME:QUALified, 2-946
- TRIGger[:SEquence]:TIME:QUALified:
TIME<x>, 2-947
- TRIGger:MASK:NEW, 2-925
- TRIGger:MASK:OPEN, 2-927
- TRIGger:MASK:SAVE, 2-928

U

UNIT:POWer, 2-948

W

*WAI, 2-948