

TEKTRONIX®

**DF 1
DISPLAY FORMATTER**

WITH OPTIONS

INSTRUCTION MANUAL

Tektronix, Inc.
P.O. Box 500
Beaverton, Oregon 97077

Serial Number _____

WARRANTY

All TEKTRONIX instruments are warranted against defective materials and workmanship for one year. Any questions with respect to the warranty should be taken up with your TEKTRONIX Field Engineer or representative.

All requests for repairs and replacement parts should be directed to the TEKTRONIX Field Office or representative in your area. This will assure you the fastest possible service. Please include the instrument Type Number or Part Number and Serial Number with all requests for parts or service.

Specifications and price change privileges reserved.

Copyright © 1976 by Tektronix, Inc., Beaverton, Oregon. Printed in the United States of America. All rights reserved. Contents of this publication may not be reproduced in any form without permission of Tektronix, Inc.

U.S.A. and foreign Tektronix products covered by U.S. and foreign patents and/or patents pending.

TEKTRONIX is a registered trademark of Tektronix, Inc.

TABLE OF CONTENTS

PAGE		PAGE
	LIST OF ILLUSTRATIONS	ii
	LIST OF TABLES	iii
	OPERATORS SAFETY INFORMATION	iv
	SERVICE SAFETY INFORMATION	v
	SECTION 1 GENERAL INFORMATION	
	INTRODUCTION	1-1
	GLOSSARY OF TERMS	1-1
	INSTALLATION	1-2
	PACKAGING FOR SHIPMENT	1-2
	SPECIFICATION	1-4
	STANDARD ACCESSORIES	1-6
	RECOMMENDED ACCESSORIES	1-7
	SECTION 2 OPERATING INSTRUCTIONS	
	CONTROLS AND CONNECTORS	2-1
	INTERNAL	2-1
	EXTERNAL	2-1
	DETAILED OPERATING INSTRUCTIONS	2-4
	POWER-ON MODE	2-4
	DISPLAY MODES	2-4
	Timing Diagram Displays	2-4
	Map	2-4
	State Table Displays	2-4
	7D01 ONLY	2-6
	7D01 ⊕ INTENS REF	2-6
	REF TABLE FOLLOWS 7D01	2-6
	REF TABLE HELD	2-6
	REF TABLE FOLLOWS WITH/OFFSET	2-7
	SEARCH	2-7
	RESET IF TABLES=	2-7
	RESET IF 7D01=REF	2-7
	STORE 7D01 → REF	2-7
	COLUMN BLANKING	2-8
	LOGIC STATES	2-8
	Size and Position Adjustm	2-8
	Error Message Displays	2-8
	FUNCTIONAL CHECK	2-9
	SETUP PROCEDURE	2-9
	TIMING DIAGRAM DISPLAY	2-9
	MAP DISPLAYS	2-9
	STATE TABLE DISPLAYS	2-10
	FRONT-PANEL ADJUSTMENTS	2-12
	SECTION 3 THEORY OF OPERATION	
	FRONT PANEL	3-1
	DATA ACQUISITION	3-1
	MPU, PROGRAM, AND DATA STORAGE	3-2
	VERT AND HORIZ DISPLAY OUTPUT	3-2
	CHARACTER MEMORY AND GENERATOR	3-3
	DISPLAY CONTROL AND Z-AXIS	3-3
	DISPLAY	3-4
	SECTION 4 MAINTENANCE	
	PREVENTIVE MAINTENANCE	4-1
	CLEANING	4-1
	VISUAL INSPECTION	4-1
	SEMICONDUCTOR CHECKS	4-1
	TROUBLESHOOTING	4-2
	TROUBLESHOOTING AIDS	4-2
	TROUBLESHOOTING EQUIPMENT	4-2
	TROUBLESHOOTING TECHNIQUES	4-3
	Troubleshooting with the System Text Fixture	4-4
	CORRECTIVE MAINTENANCE	4-14
	OBTAINING REPLACEMENT PARTS	4-14
	SOLDERING TECHNIQUES	4-14
	COMPONENT REMOVAL AND REPLACEMENT	4-15
	Circuit Boards	4-15
	Pushbutton Switches	4-18
	Semiconductors	4-18
	Interconnecting Pins	4-19
	ADJUSTMENT AFTER REPAIR	4-20
	SECTION 5 PERFORMANCE CHECK AND ADJUSTMENT	
	PRELIMINARY INFORMATION	5-1
	Adjustment Interval	5-1
	Tektronix Field Service	5-1
	Performance Check	5-1
	Adjustment Procedure	5-1
	Partial Procedure	5-1
	TEST EQUIPMENT REQUIRED	5-2
	INDEX TO PERFORMANCE CHECK AND ADJUSTMENT	5-3
	PRELIMINARY PROCEDURE	5-3
	PERFORMANCE CHECK PROCEDURE	5-4
	ADJUSTMENT PROCEDURE	5-8
	SECTION 6 REPLACEABLE ELECTRICAL PARTS	
	SECTION 7 INSTRUMENT OPTIONS	
	SECTION 8 DIAGRAMS AND CIRCUIT BOARD ILLUSTRATIONS	
	SECTION 9 REPLACEABLE MECHANICAL PARTS	
	CHANGE INFORMATION	

WARNING

THE REMAINING PORTION OF THIS TABLE OF CONTENTS LISTS THE SERVICING INSTRUCTIONS. THESE SERVICING INSTRUCTIONS ARE FOR USE BY QUALIFIED PERSONNEL ONLY. TO AVOID ELECTRICAL SHOCK, DO NOT PERFORM ANY SERVICING OTHER THAN THAT CALLED OUT IN THE OPERATING INSTRUCTIONS UNLESS QUALIFIED TO DO SO.

LIST OF ILLUSTRATIONS

FIGURE NO.	PAGE	FIGURE NO.	PAGE
Frontis- piece	DF1 Featuresvi	4-10	Exploded view of circuit-board pin and ferrule 4-20
1-1	Attaching the DF1 to the 7D01.1-3	5-1	Location of 7D01 Full Display/First Trigger jumper . . 5-4
1-2	DF1 dimensional drawing1-5	5-2	Test setup for Performance Check and Adjustment Procedure 5-5
2-1	Location of the Readout Source multi-pin jumper . . . 2-1	5-3	Hexadecimal State Table display 5-6
2-2	Front-panel controls, connectors, and indicators . . . 2-2	5-4	Reset Out check test setup. 5-7
2-3	Typical DF1 Display Modes 2-5		
2-4	Typical map display usage 2-6		
2-5	Typical state-table display showing offset between the 7D01 and reference state tables. 2-7		
2-6	Test setup for Functional Check procedure 2-10		
2-7	Typical map display of 16 channels from the 067-0804-00 Interface Test Fixture 2-11		
2-8	Typical map display of 15 channels from the 067-0804-00 Interface Test Fixture (channel 5 input disconnected). 2-11		
4-1	Test equipment setup for troubleshooting the DF1 Digital Formatter 4-5		
4-2	Partial view of Intelligence circuit board. Shows pin location and indexing for connection to the Interface Test Fixture 4-5	8-1	Semiconductor lead configurations.
4-3	Location of readout source multi-pin jumper 4-9	8-2	Circuit board locations.
4-4	Circuit board locations 4-16	8-3	A1—Formatter Keyboard circuit board locations as viewed from front of instrument.
4-5	Locations of securing screws on the front sub-panel . . 4-17	8-4	A2—Button Lights circuit board component locations as viewed from the component side of the board.
4-6	Locations of securing screws on A2 Button Lights circuit board. 4-17	8-5	A4—Acquisition circuit board component locations.
4-7	Locations of hex securing spacers and wiring to be disconnected on A1 Formatter Keyboard circuit board. 4-18	8-6	A3—Intelligence circuit board component locations.
4-8	Locations of securing screws on A3 Intelligence circuit board. 4-18	8-7	Partial A4—Acquisition circuit board. Component loca- tions as viewed from component side of the board.
4-9	Locations of securing screws and hardware mounting screws on A4 Acquisition circuit board 4-19	8-8	A4—Acquisition circuit board component locations.
		8-9	A3—Intelligence circuit board component locations.
		8-10	A4—Acquisition circuit board component locations.
		8-11	Partial A3—Intelligence circuit board. Component loca- tions as viewed from the component side of the board.
		8-12	Partial A4—Acquisition circuit board. Component loca- tions as viewed with board installed.
		8-13	Partial A3—Intelligence circuit board component locations.

The illustrations in Section 8 are located near their associated diagrams on the foldout pages.

LIST OF TABLES

TABLE NO.		PAGE	TABLE NO.		PAGE
1-1	Electrical Characteristics	1-4	4-4	Keyboard Circuit Checkout Procedure	4-7
1-2	Environmental Characteristics	1-5	4-5	Manual Clock Pulses Required To Control Button Lights	4-8
1-3	Physical Characteristics	1-5	4-6	Formatter Readout Truth Table	4-9
3-1	Data Acquisition Address Decoder	3-1	4-7	Mainframe Readout Truth Table	4-10
4-1	Error Messages and Responses	4-2	5-1	Performance Check Description	5-1
4-2	Hex-to-Binary Conversion	4-6	5-2	Test Equipment	5-3
4-3	ROM Hexadecimal Output Program	4-7			

OPERATORS SAFETY INFORMATION

The following general safety information is provided to ensure safe operation of this instrument and applies to all operators and service personnel. Specific warnings will be found throughout the manual where they apply and should be followed in each instance.

WARNING statements identify conditions or practices which could result in personal injury or loss of life.

CAUTION statements identify conditions or practices which could result in damage to the equipment or other property.

The word **DANGER** on the equipment identifies areas of immediate hazard which could result in personal injury or loss of life.

The following safety symbols may appear on the equipment:



CAUTION—Refer to manual



DANGER—High voltage



Protective ground (earth) terminal

Other warning symbols where they apply.

WARNING

Ground the Instrument

To reduce electric-shock hazard, the mainframe (oscilloscope) chassis must be properly grounded. Refer to the mainframe manual for grounding information.

Do Not Operate in Explosive Atmosphere

Do not operate this instrument in an area where flammable gases or fumes are present. Such operation could cause an explosion.

Do Not Remove Instrument Covers

To avoid personal injury, do not operate the instrument without covers installed. Do not perform any servicing other than that contained in the Operators Manual unless you are qualified to do so.

Do Not Service or Adjust Alone

Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

CAUTION

Prevent Instrument Damage

To prevent instrument damage, plug-in units should not be installed or removed without first turning off the mainframe power.

SERVICE SAFETY INFORMATION

The following are safety precautions which appear in the servicing information sections of this manual. This Service Safety Information is in addition to the Operators Safety Information given previously.

WARNING

Disconnect Instrument Power

To avoid electric shock, disconnect the instrument from the power source before soldering or replacing components.

CAUTION

Use Proper Cleaning Agents

Avoid the use of chemical cleaning agents which might damage the plastics used in this instrument. Use a non-residue type of cleaner, preferably isopropyl alcohol, total denatured ethyl alcohol, or TP35. Before using any other type of cleaner, consult your local Tektronix Service Center or representative.

Exercise Care When Checking Diodes


Do not use the ohmmeter on a scale that has high internal current. High currents may damage the diode.

Exercise Care When Soldering on Multi-layer Boards

The Acquisition, Intelligence, and Button Lights circuit boards in this instrument are multi-layer type boards with a conductive path(s) laminated between the top and bottom board layers. All soldering on these boards should be done with extreme care to prevent breaking the connections to the center conductor(s); only experienced maintenance personnel should attempt repair of these boards.

Do Not Use Pin Sockets for Connection Points

The spring tension of the pin sockets ensures a good connection between the circuit board and the pin. This spring tension can be destroyed by using the pin sockets as a connecting point for spring-loaded probe tips, alligator clips, etc.

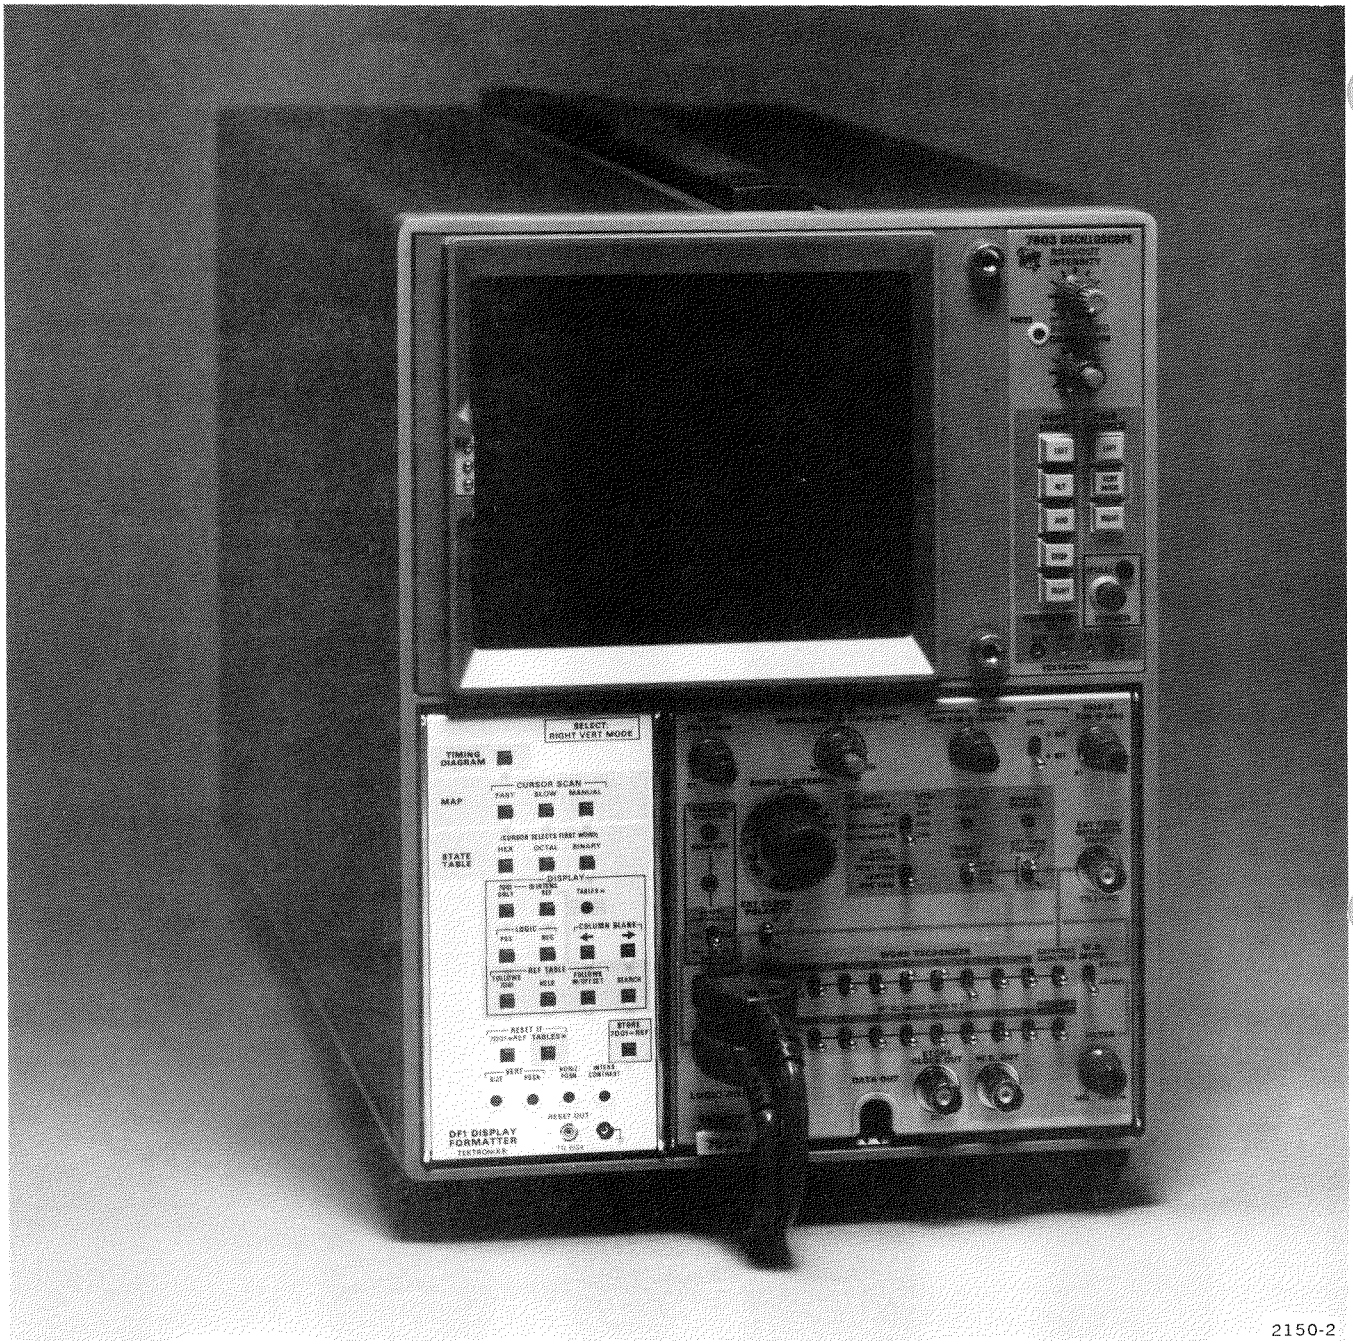

2150-2

DF1 FEATURES

The DF1 Display Formatter provides data-domain display modes in addition to the existing time-domain display of the 7D01 Logic Analyzer. It adds state table displays with a comparison mode, and a map display. The DF1 attaches to the left side of the 7D01, forming a three-wide plug-in assembly. This assembly operates in a 7000-series oscilloscope mainframe to comprise a complete 16-channel logic timing-state analyzer system.

A microprocessor controlled memory system, contained in the DF1, is capable of recording two 7D01 information records. Portions of both information records may be displayed concurrently in a state table presentation.

State tables are displayed in terms of either hexadecimal, octal, or binary formats. This data may be displayed in up to two tables of 17 lines of 16-bit words each. The left-hand table displays data currently stored in the 7D01 memory (7D01 display). The right-hand table displays data that has been transferred from previous 7D01 displays to the DF1 memory (reference display). The DF1 compares the 2 tables and resets the 7D01 when the 7D01 data equals the reference data.

The map function plots a dot display of the 16 data channels in X-Y coordinate points. Each dot location represents one possible combination of up to 16 inputs to the 7D01

GENERAL INFORMATION

INTRODUCTION

The Operator's Manual contains information necessary to effectively operate the DF1 Display Formatter unit and is divided into three sections: Section 1 provides packaging for shipment information, specifications, and a list of standard accessories. Section 2 contains operating information. Information concerning available options is located in Section 3.

The Instruction Manual contains nine sections. Operating information is covered in the first two sections; servicing information is covered in the remaining seven sections. Schematic diagrams are located at the rear of the manual and can be unfolded for reference while reading other parts of the manual. The reference designators and symbols used on the schematic diagrams are defined on the first page of the Diagrams and Circuit Board Illustrations section. Abbreviations used in the manuals, except in the parts list and schematic diagrams, comply with the American National Standards Institute Y1.1-1972 publication. The parts list is a computer printout and uses computer-supplied abbreviations.

GLOSSARY OF TERMS

The following logic terms are used throughout this manual.

Asynchronous Mode—The data is acquired by the 7D01 using its internal clock at a rate selected by its sample interval control.

Bit—The smallest increment of digital information.

Blanked Columns—The columns eliminated from the memory by the COLUMN BLANK function.

Compare—A check between the 7D01 memory and the reference memory for equality (a microprocessor function.)

Data—This is information acquired by the 7D01. Up to 16 channels of data may be acquired, and each data bit is one clock period in the synchronous mode.

Data Record—All of the information stored in the 7D01 memory or the DF1 memory. (A Data Record has 4096 bits of information.)

Data Word—This is Good Data that may be formatted in any of three different ways:

1. A vertical slice of the Timing Diagram display.

2. A coordinate point of the Map display.
3. A horizontal line of characters in a State Table display.

NOTE

Channel 0 is the top-most channel displayed in TIMING DIAGRAM format and is always considered the least significant bit.

Don't Care Data—Invalid Data that is excluded from comparison in all comparison modes.

End Data—Data that fills out the last portion of a table when valid data ends before completion of the table. This is indicated by an "*" in the display.

Good Data—All data which is not Invalid Data.

Indeterminate Data—This is valid data but is considered invalid because its location cannot be defined. This data is indicated by an "X" in the display and occurs during sweep retrace in Timing Diagram. The number of Indeterminate Data bits for each position of the 7D01 bits/channel switch are: Two bits (254 bits/channel position), four bits (508 bits/channel position), and eight bits (1016 bits/channel position).

Invalid Data—This term describes a combination of Indeterminate Data, Old Data (if any), and End Data.

New Data—The most recent acquisition of Good Data into the 7D01.

Old Data—Data which was part of a previous Data Record in the 7D01 memory but is out of sequence. This is caused by the arrival of the trigger before the New Data has completely filled the memory. Old Data is indicated by an "X" in the display.

Reference State Table—A display of DF1 memory data transferred from a previous 7D01 display and displayed on the right half of the crt.

Synchronous Mode—The data is acquired by the 7D01 using an externally supplied clock signal (7D01 sample interval switch set to external, and with the external clock signal connected to the clock input of the channel 0-7 Data Acquisition Probe).

Word—See Data Word.

INSTALLATION

The DF1 Display Formatter attaches to the left side of the 7D01 Logic Analyzer to make a three-wide plug-in system. The two units latch together to provide a rigid instrument that plugs into a 7000-series mainframe. Refer to Figure 1-1 to attach the DF1 to the 7D01.

CAUTION

To prevent instrument damage, plug-in units should not be installed or removed without first turning off the mainframe power.

To install the DF1/7D01, first turn off the power to the oscilloscope mainframe. Then, gently push the 2 plug-in units into the appropriate plug-in compartments until they fit firmly. The front panels of the DF1/7D01 should be flush with the front panel of the oscilloscope mainframe.

NOTE

When installed in a four-compartment mainframe, the DF1/7D01 occupies the left vertical, right vertical, and A horizontal compartments only. The oscilloscope mainframe vertical mode switch must be set to right and the horizontal mode switch must be set to A.

To remove the DF1/7D01, pull the release latch (located on the lower left corner of the 7D01) to disengage the DF1/7D01 from the mainframe. Then, gently slide the plug-in units from the mainframe.

PACKAGING FOR SHIPMENT

If this instrument is to be shipped for long distances by commercial transportation, it is recommended that the instrument be packaged in the original manner for maximum protection. The carton and packaging material in which your instrument was shipped should be saved and used for this purpose.


Also, if this instrument is to be shipped to a Tektronix Service Center for service or repair, attach a tag to the instrument showing the following: Owner of the instrument (with address), the name of an individual at your firm that can be contacted, complete instrument type and serial number, and a description of the service required.

If the original packaging is unfit for use or not available, package the instrument as follows:


1. Obtain a carton of corrugated cardboard with at least a 200-pound test strength and at least 6 inches larger than the instrument dimensions to allow for cushioning.
2. Surround the instrument with polyethylene sheeting to protect the instrument.
3. Allow a 3-inch cushion on all sides by tightly packing dunnage or urethane foam between the carton and the instrument.
4. Seal the carton with shipping tape or with an industrial stapler.
5. Mark the address of the Tektronix Service Center and your return address on the carton in one or more locations.

DF1/7D01 INSTALLATION


- 1 Slide the movable latch on the top of the DF1 forward until it stops.

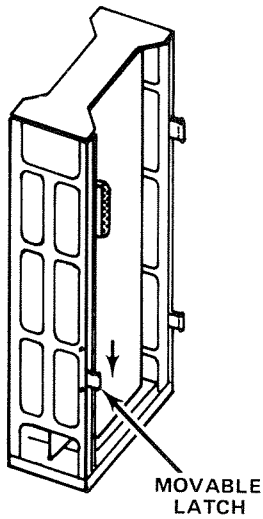


- 2 Tilt the DF1 and 7D01 slightly and place the bottom two latches on the DF1 into the bottom two slots on the 7D01. Gently slide the DF1 forward to just engage the bottom latches with the bottom track on the 7D01.

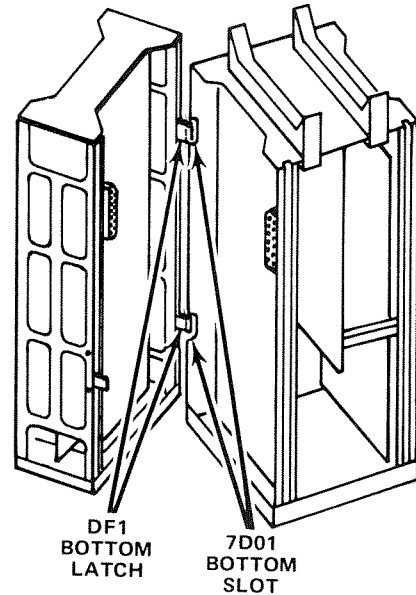

- 3 Continue to slide the DF1 forward until the jack at the top rear of the DF1 lines up with its mating plug on the 7D01.

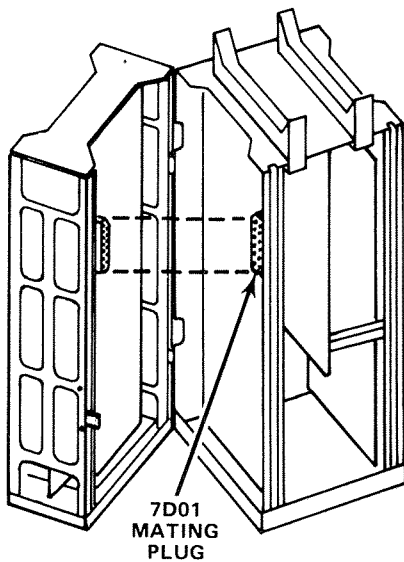

- 4 Gently press the units together until the connector is properly mated and the movable latch is inserted into the rail slot on the 7D01.

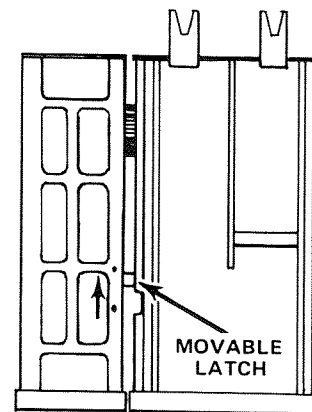

Make sure the movable latch fits into the 7D01 rail groove and slide the movable latch toward the rear along the rail groove until it stops. The DF1 and 7D01 should now be latched together to form a rigid three-wide plug-in system.

2150-10

Figure 1-1. Attaching the DF1 to the 7D01.

SPECIFICATION

The electrical specifications listed in Table 1-1 apply for the DF1/7D01 system under the following conditions: (1) The instrument must have been adjusted at an ambient temperature between +20° and +30° C (+68° to +86° F), (2) the instrument must be operating in an ambient temperature between 0° and +40° C (+32° and +104° F), and (3) the instrument must have been operating for at least 20 minutes.

TABLE 1-1
Electrical Characteristics

Characteristic	Performance Requirement
External Read Clock	
Frequency Range	100 kHz to 500 kHz.
Duty Cycle	50% within 5%.
Display	
Vertical Size	Adjustable from 6.9 div or less to at least 8.1 div from the top of the first line of DF1 readout to the bottom of the last line of DF1 readout.
Vertical Position	Adjustable to vertical center of display area in any calibrated 7000-series mainframe.
Horizontal Position	Adjustable to horizontal center of display area in any calibrated 7000-series mainframe.
Output Signals	
Reset Logic Voltage Level	LO: +0.4 V or less at 2 mA. HI: at least +2.4 V at 2 mA.
Waveshape	Positive-going rectangular pulse.
Duration	100 μ s within 50 μ s when used with the 7D01 internal read clock.

TABLE 1-2
Environmental Characteristics

Characteristic	Performance Requirement
Temperature	
Calibration	+20° to +30° C (+68° to +86° F).
Operating	0° to +40° C (+32° to +104° F).
Storage	-55° to +75° C (-67° to +167° F).
Altitude	
Operating	To 15,000 feet.
Storage	To 50,000 feet.
Transportation	Qualified under National Safe Transit Committee Test Procedure 1A, Category II.

TABLE 1-3
Physical Characteristics

Characteristic	Description
Net Weight	Approximately 2 lbs (0.9 kg).
Overall Dimensions	See Figure 1-2, Dimensional Drawing.

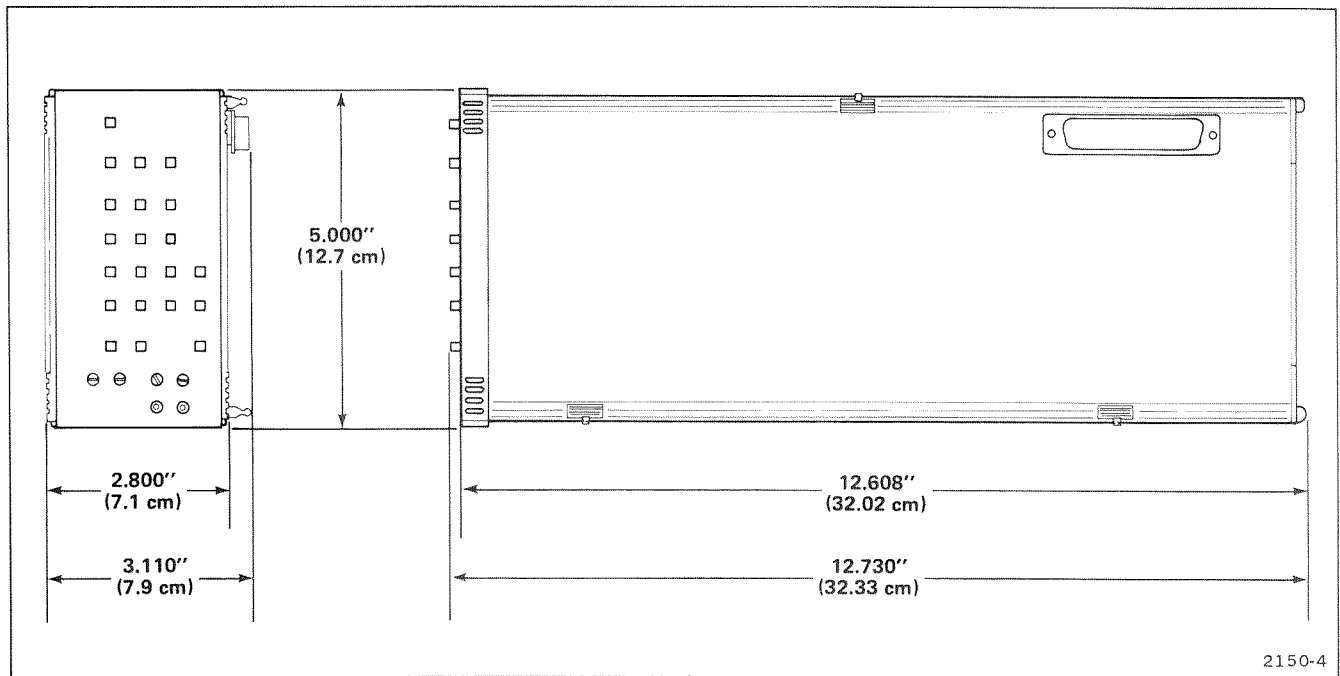


Figure 1-2. DF1 dimensional drawing.

STANDARD ACCESSORIES

- 1 eaOperators Manual
- 1 ea Instruction Manual

Refer to the tabbed Accessories page in the back of this manual for standard accessory part numbers.

RECOMMENDED ACCESSORIES

The following accessories have been selected from our catalog specifically for your instrument. They are listed as a convenience to help you meet your measurement needs. For detailed information and prices, refer to a Tektronix Products Catalog or contact your local Tektronix Field Representative.

CABLE

TWO-PIN TO BNC: This adapter-cable connects the output gate and ground pin-jacks on the DF1 front panel to an external application.


Cable, Order 175-1178-00




CAMERA

C-5A: The C-5A is a low-cost general-purpose camera with a Polaroid Pack-Film Back, pulsed graticule illumination, and a fixed f/16 lens. Magnification may be set at 0.67 or 0.85.

Order C-5A

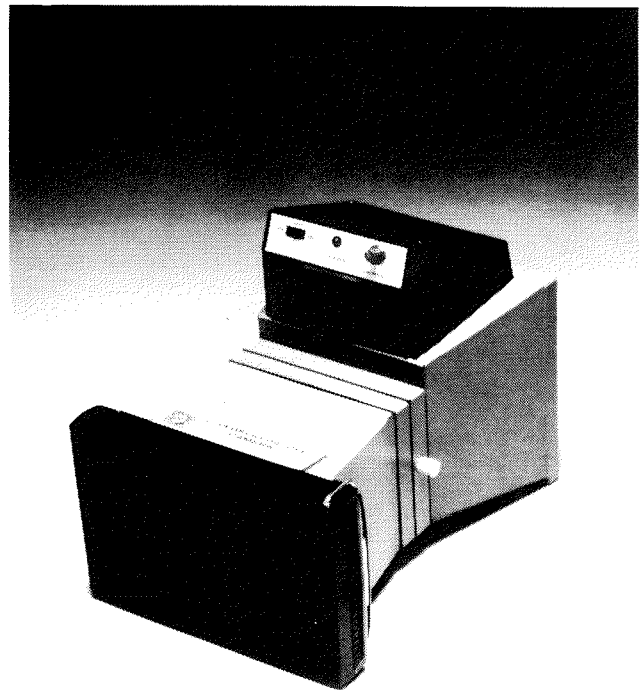

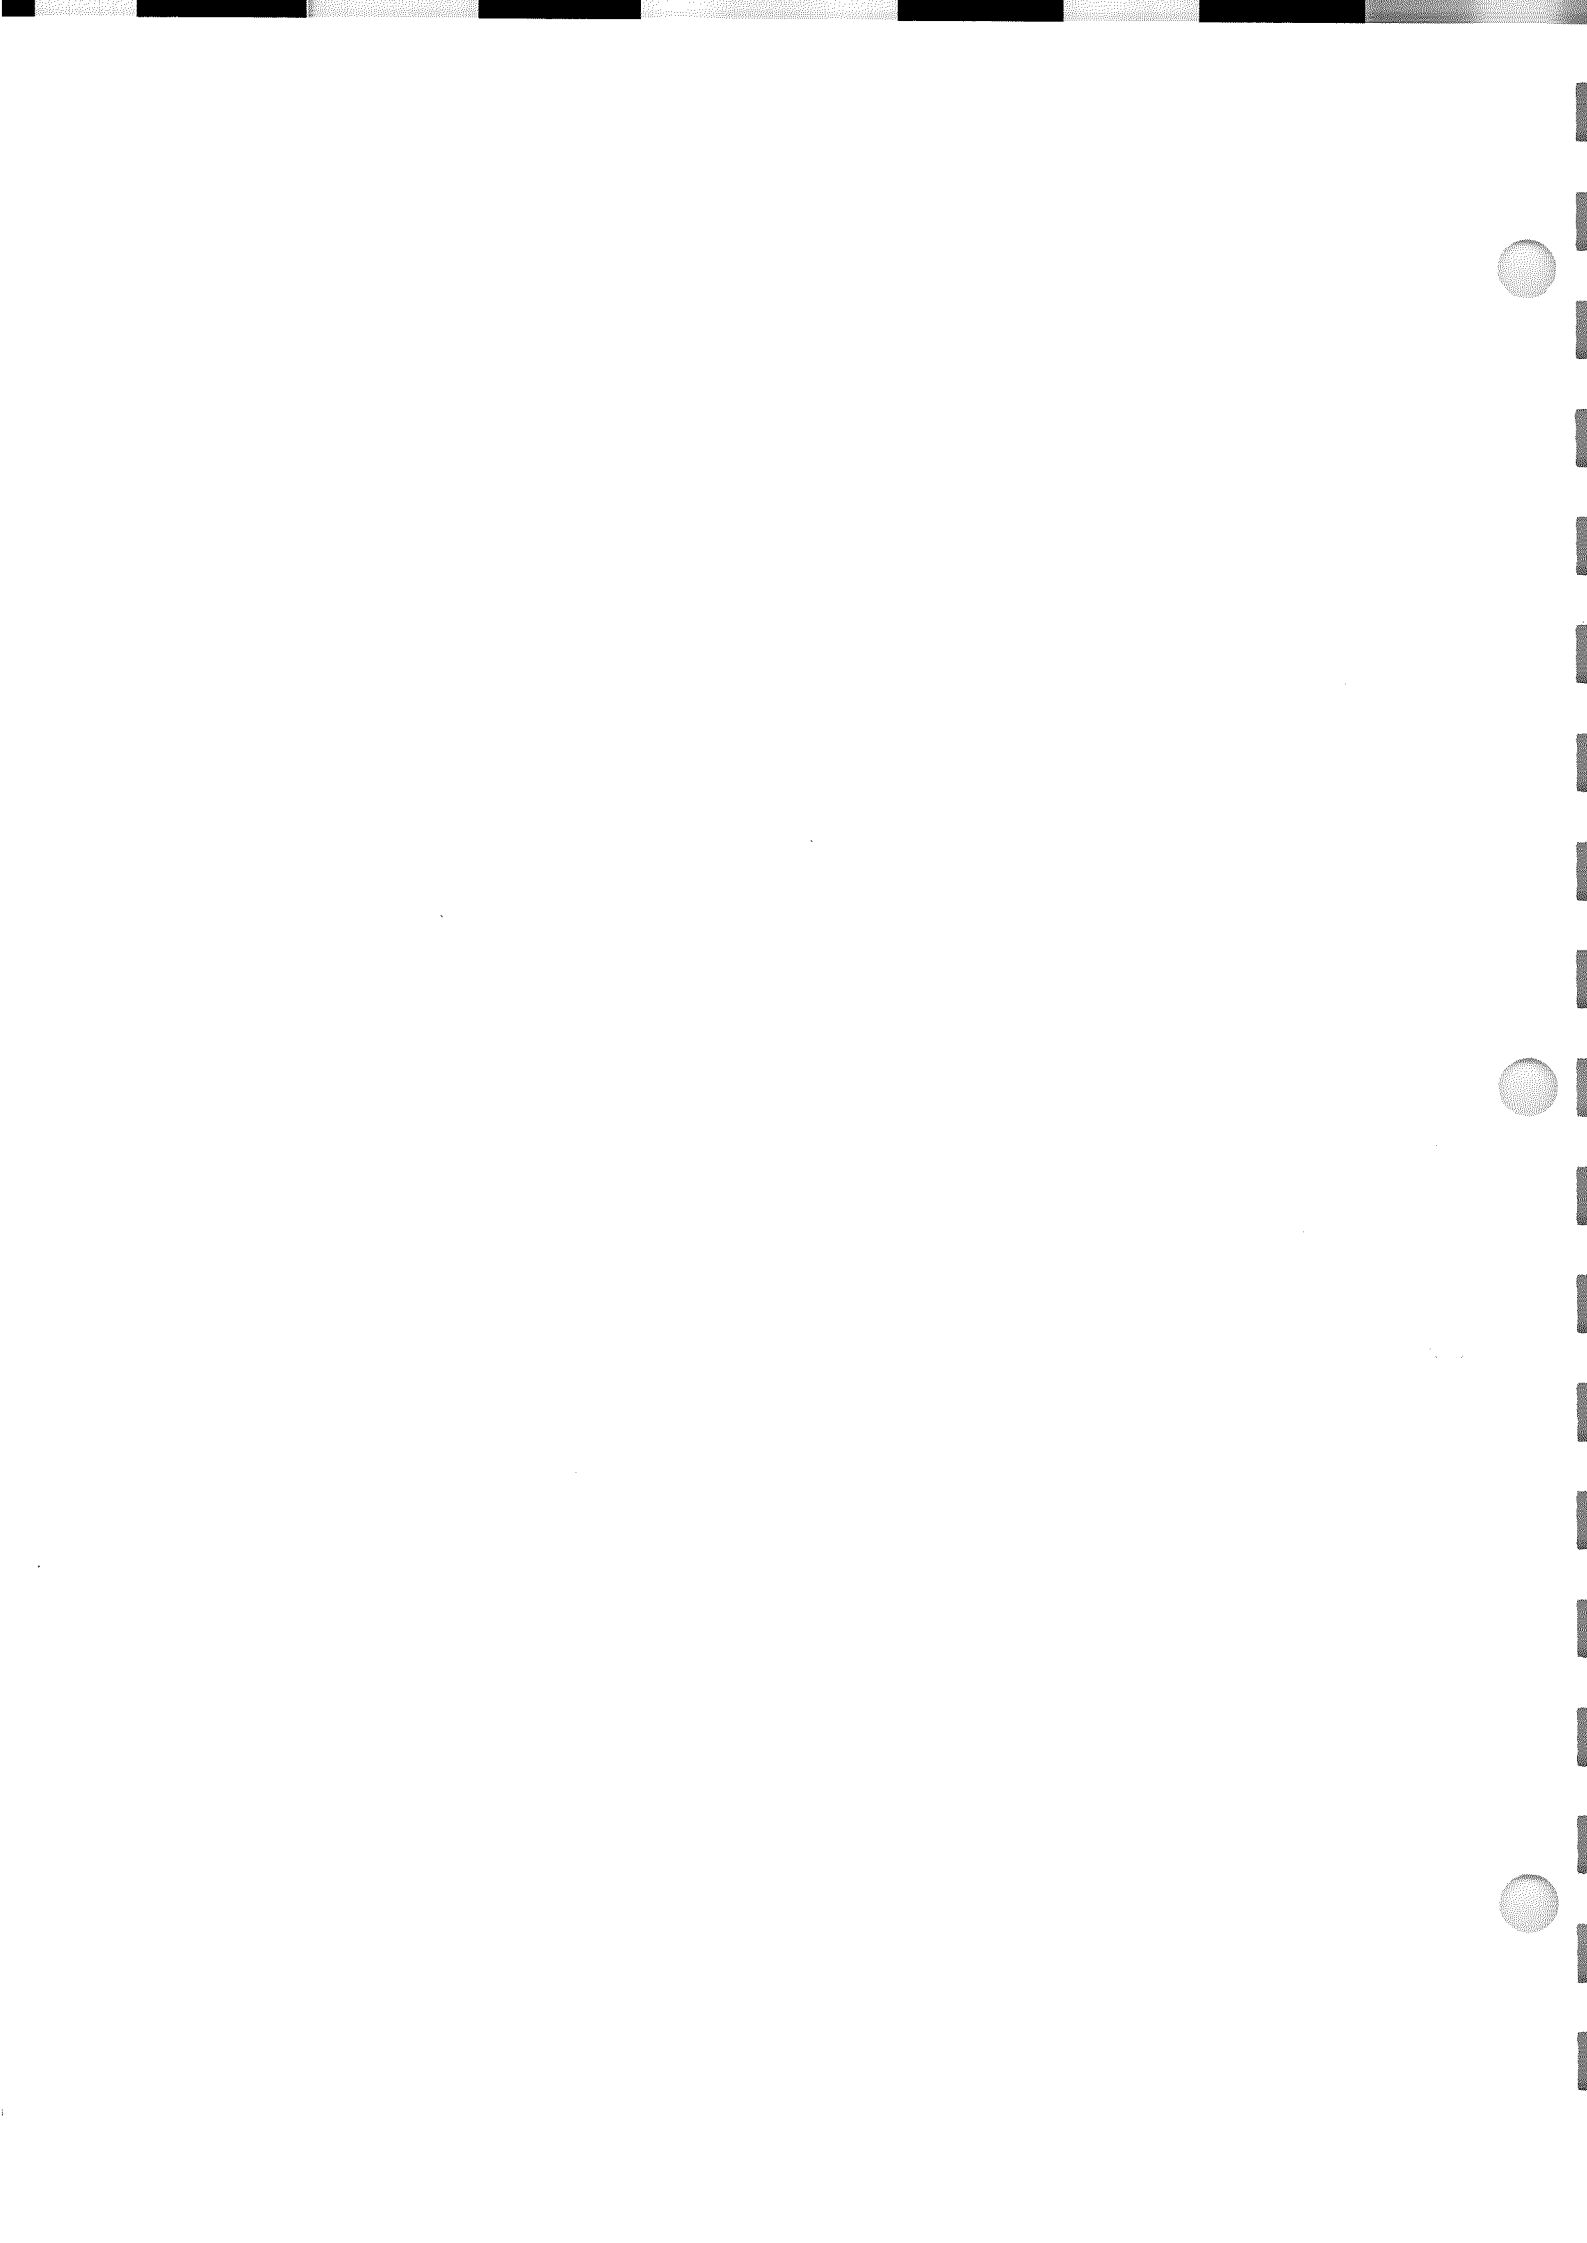

OPERATING INSTRUCTIONS

To effectively use the DF1 Display Formatter, the capabilities of the DF1 and the companion 7D01 Logic Analyzer must be known. This section briefly describes the operation of the controls and connectors, provides detailed operating instructions, and a functional check procedure for the DF1. The General Information section provides instructions for installation of the DF1 and the 7D01 into a 7000-series oscilloscope mainframe. Refer to the 7D01 Operators or Instruction Manuals for information on the 7D01 Logic Analyzer.

CONTROLS AND CONNECTORS

INTERNAL

The Readout Source jumper is located inside the DF1. When using the Timing Diagram display, readout can be produced either by the DF1 readout system or by the readout system of the associated oscilloscope mainframe (refer to Figure 2-1). We recommend using the DF1 readout unless it is important to have the style of characters produced by the mainframe readout system.

EXTERNAL

The major controls required for operation of the DF1 are located on the front panel of the unit. Figure 2-2 provides a brief description of the front-panel functions. More information is given under Detailed Operating Instructions.


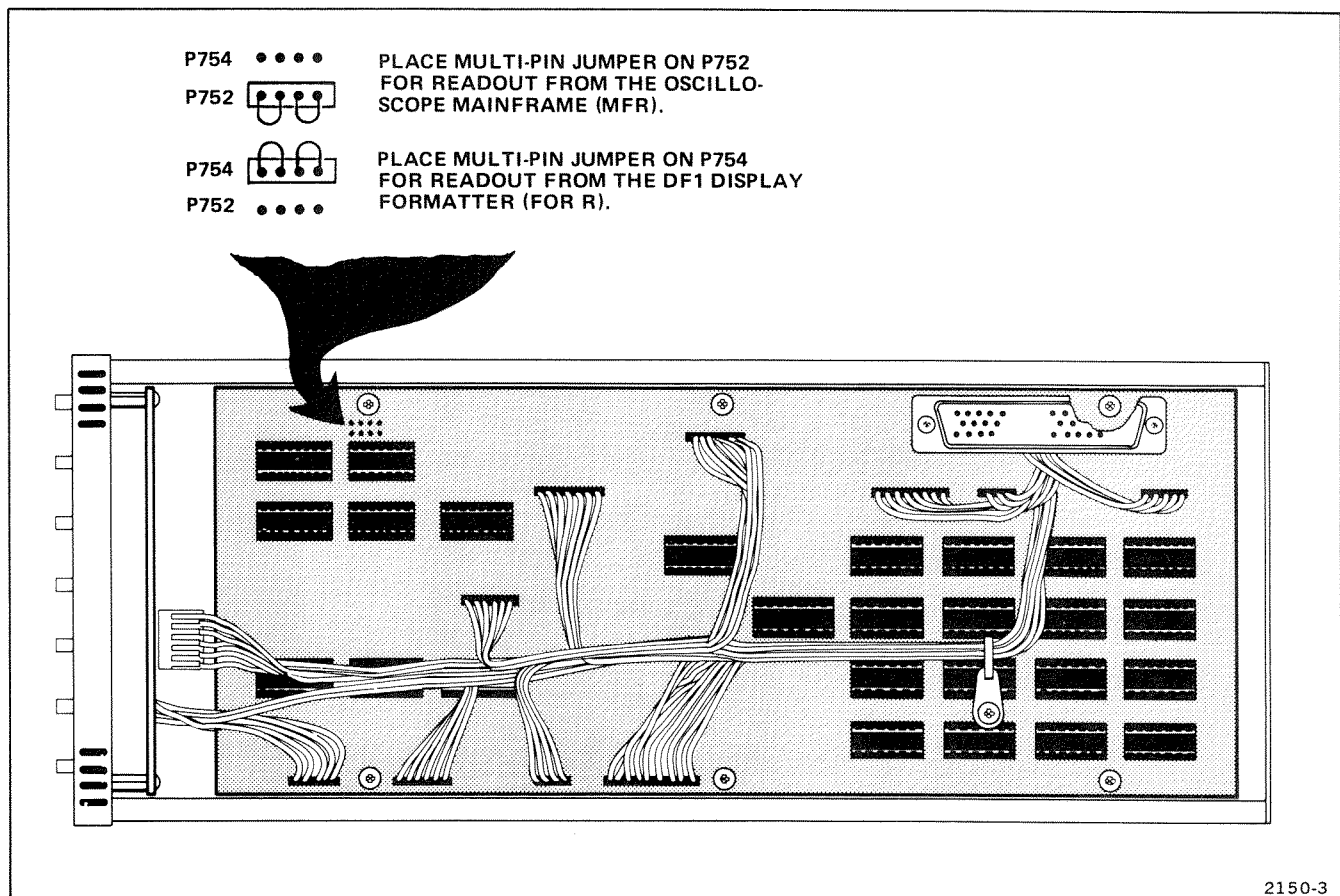


Figure 2-1. Location of the Readout Source multi-pin jumper.

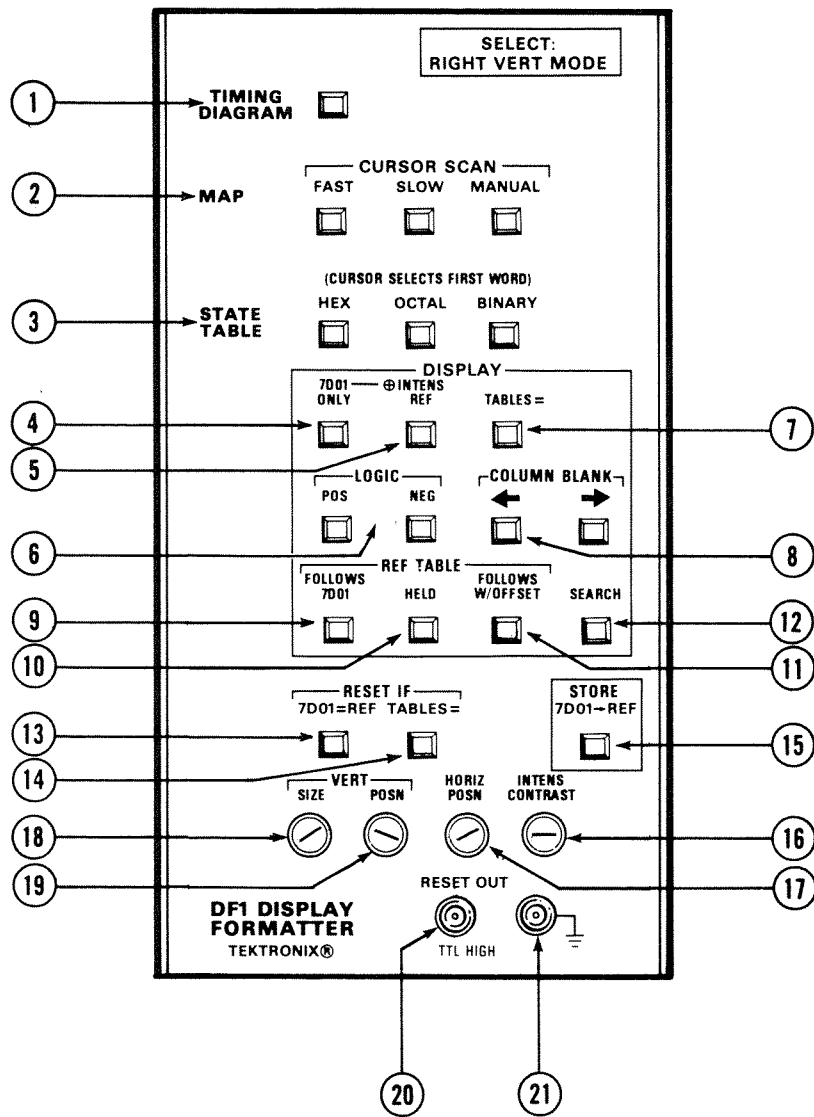

2150-1A

Figure 2-2. Front-panel controls, connectors, and indicators.

- 1 **Timing Diagram Switch**—Selects the timing diagram display from the 7D01 Logic Analyzer.
- 2 **MAP (CURSOR SCAN Switches)**—Select view of the 7D01 memory data in X-Y coordinate points on the oscilloscope mainframe crt. The DF1 automatically sequences the data locations at a FAST or SLOW rate, or data locations are selected manually with the 7D01 Cursor control.
- 3 **STATE TABLE Switches**—Select tabular display of the cursor word, the 16 words following the cursor word, and the trigger word. The tabular format can be displayed in HEX (hexadecimal), OCTAL, or BINARY base-number systems.
- 4 **7D01 ONLY Switch**—Selects the state table from the 7D01 memory for display on the left-hand side of the crt.
- 5 **⊕(Exclusive Or) INTENS REF Switch**—Compares state table display from the 7D01 memory (left-hand column) to a reference state table stored by the DF1 (right-hand column).
- 6 **LOGIC Switches**—Determine whether the state table displays are in positive or negative logic.
- 7 **TABLE = Indicator**—Lamp turns on when the 7D01 state table and the reference state table are equal.
- 8 **COLUMN BLANK Switches**—Provide column blanking for state table displays. The blanked columns are excluded from the data base for all state table comparison and reset functions.
- 9 **REF TABLE FOLLOWS 7D01 Switch**—The cursor location (trigger-to-cursor difference) in the reference state table (right-hand column) follows the cursor location in the 7D01 state table (left-hand column).
- 10 **REF TABLE HELD Switch**—Locks the cursor location in the reference state table which allows the cursor location in the 7D01 reference state table to be moved independently.
- 11 **REF TABLE FOLLOWS W/OFFSET Switch**—Maintains the cursor location offset, between the 7D01 and reference state tables, that was established in the REF TABLE HELD mode.
- 12 **SEARCH Switch**—The 7D01 memory is searched for a match of the cursor word (first word) in the reference state table.
- 13 **RESET IF 7D01 = REF Switch**—The 7D01 memory is reset when the 7D01 memory equals the DF1 reference memory.
- 14 **RESET IF TABLES = Switch**—The 7D01 memory is reset when the 7D01 state table display equals the reference state table display.
- 15 **STORE 7D01 → REF Switch**—Transfers the 7D01 memory into the DF1 reference memory.
- 16 **INTENS CONTRAST Adjustment**—Controls brightness of the intensified characters of the DF1 display.
- 17 **HORIZ POSN Adjustment**—Controls horizontal position of the DF1 display.
- 18 **VERT SIZE Adjustment**—Varies vertical size of the DF1 display.
- 19 **VERT POSN Adjustment**—Controls vertical position of the DF1 display.
- 20 **RESET OUT Connector**—Pin-jack connector provides a HIGH TTL level output when the 7D01 memory is reset by the DF1.
- 21 **Ground Connector (⊥)**—Pin-jack connector provides a ground return for the RESET OUT gate.

2150-1B

Figure 2-2. Front-panel controls, connectors, and indicators (continued).

DETAILED OPERATING INSTRUCTIONS

POWER-ON MODE

When power is applied to the oscilloscope mainframe (Power-On mode), the DF1 reference memory and the memory which acquires data from the 7D01 are checked for proper operation of the random access memory (RAM) integrated circuits (refer to Error Message Displays in this section). Then, the 7D01 is reset and the DF1 reference memory and the 7D01 memory are cleared. The Display Mode is automatically set to Timing Diagram, the LOGIC is set to POS, and the cursor location (trigger-to-cursor readout) is set to +0. All other DF1 push-button selections are cancelled.

DISPLAY MODES

The DF1 displays digital data in 3 Display Modes: Timing Diagram, Map, and State Table. Figure 2-3 shows the controls required to activate typical DF1 displays.

Timing Diagram Displays

The front-panel TIMING DIAGRAM push button selects the Timing Diagram display (4, 8, or 16 channels) from the companion 7D01 Logic Analyzer (see Fig. 2-3). The cursor function of the 7D01 provides an intensified zone on the data display and a corresponding numerical readout display shows the logic state for each displayed channel of data. The position of the cursor, relative to the trigger, is also displayed on the crt readout. Refer to the 7D01 manual for more information on the 7D01 Logic Analyzer.

The source of the display readout can be from the oscilloscope mainframe readout system (MFR) or the DF1 (FOR R). (Refer to Internal Controls and Connectors, in this section, for more information.) When the Timing Diagram Display Mode is selected (Readout Source jumper set to Formatter Readout) after either the HEX, OCTAL, or BINARY State Table function has been displayed, the cursor word readout is displayed in the same base-number system as displayed previously in the State Table Display Mode. Then, the cursor word readout changes between binary and the base-number system in the previously selected State Table Display Mode, with every other push of the TIMING DIAGRAM push button. However, if the Readout Source jumper is set for mainframe readout (MFR), cursor word readout is displayed only in the binary system.

Map

The Map function provides a view of the 7D01 memory displayed as x-y coordinate dots on the crt. The vertical axis represents the most significant half of the data word and the horizontal axis represents the least significant half (see Figure 2-3).

The map display can be formatted from 4, 8, or 16 channels of input data. Therefore, 4- and 8-channel map displays are plotted over the entire crt display area in the same manner as a 16-channel display. A 16-channel display is capable of 64,000 coordinate points, an 8-channel display is capable of 256 coordinate points, and a 4-channel display is capable of 16 coordinate points.

A map cursor, indicated by a plus symbol (+), sequences automatically through the data locations in the order in which the data was loaded into memory. The cursor scans at a FAST or SLOW rate, as determined by the CURSOR SCAN push buttons. When either the FAST or SLOW push button is held in, the cursor scan is stopped near a desired location on the display and can be positioned to the exact location with the 7D01 cursor position controls. Also, when the MANUAL CURSOR SCAN push button is pressed, the 7D01 cursor position controls are used to manually position the cursor to the exact position desired. The readout display shows the logic state of the cursor word (bottom of crt), and the position of the cursor point, relative to the trigger point, is displayed at the top of the crt.

The map display is particularly useful for a fast overall check of digital systems. First of all, the map display pattern for a particular set of digital inputs must be known. Then, if there is a change in any one of the input signals, the map display pattern will change. A different map display pattern indicates that the circuits are not operating in the normal manner. Figure 2-4 illustrates a map display pattern from 16 signal inputs and shows that the map display pattern changes when input signals are removed.

State Table Displays

The State Table function enables the data, recorded in the 7D01, to be displayed in a tabular format. The cursor word, the sixteen words which follow, and the trigger word are

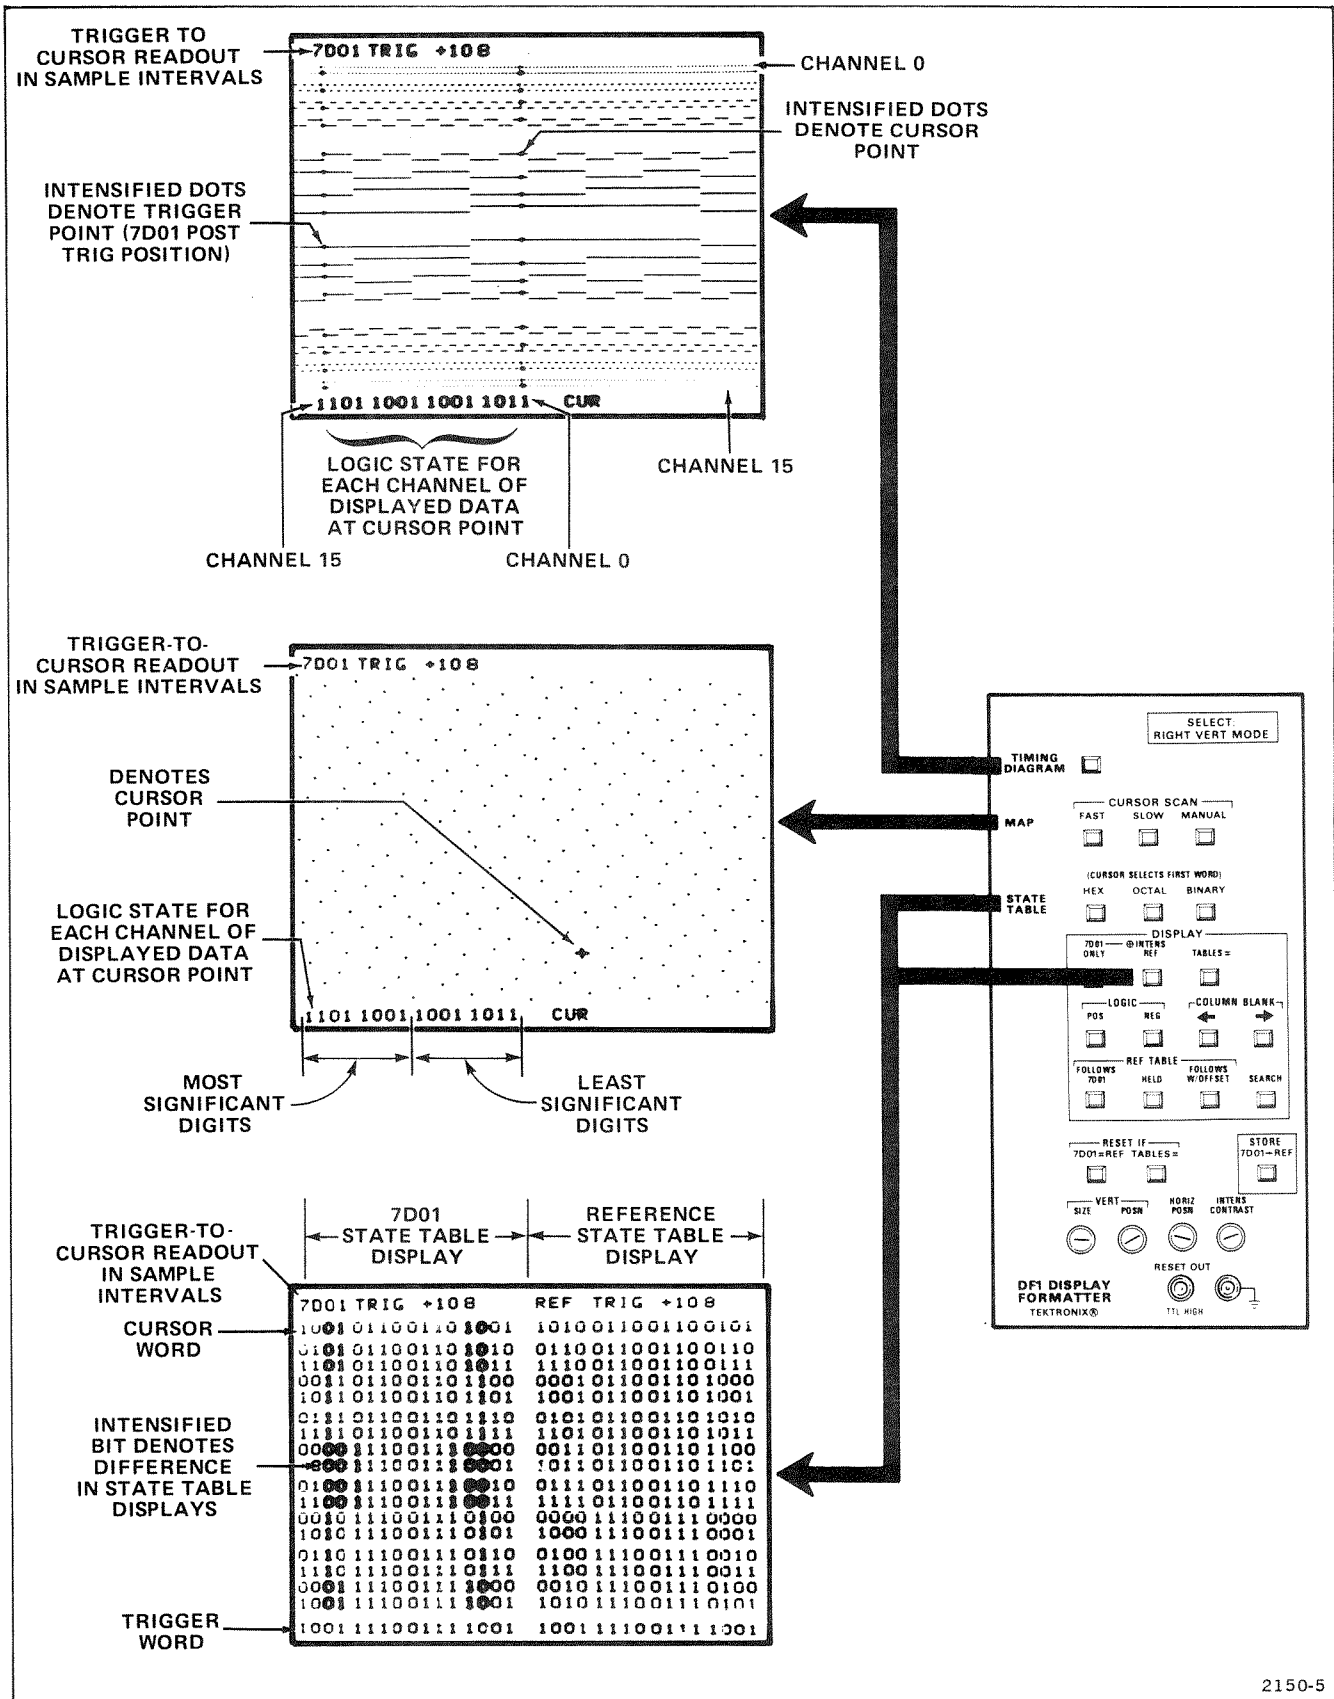


Figure 2-3. Typical DF1 Display Modes.

2150-5

displayed. If the trigger word is displayed in the first 17 words of the state table, it is indicated by a blinking condition. The position of the cursor, relative to the trigger, is also displayed on the crt readout (see Figure 2-3).

Each time the 7D01 cursor position is changed or the 7D01 is reset, the display is updated. If the data ends before 17 words are displayed, the remainder of the display is filled with an asterisk (*) character. Any "old data" from the 7D01 memory is indicated by an "X" character.

Three push-button switches select State Table displays in HEX (hexidecimal, base 16), OCTAL (base 8), or BINARY (base 2) codes. The digits are grouped in threes or fours depending upon the setting of the 7D01 cursor byte switch.

7D01 ONLY. The State Table display from the 7D01 is displayed on the left side of the crt. The \odot INTENS REF displays are not functional in the 7D01 ONLY mode.

7D01 \odot INTENS REF. Two state tables are displayed simultaneously on the crt. The state table from the 7D01 is displayed on the left half of the crt and a reference state table is displayed on the right half of the crt (see Figure 2-3). When the 7D01 \odot INTENS REF is initially selected, the STORE 7D01 \rightarrow REF push button must be pressed to load the reference memory. Any differences between the 7D01 and reference state tables are indicated by intensified bits at the appropriate location in the 7D01 state table. Any differences in the state tables due to old data, indeterminate data, end data, or blanked columns, is interpreted as "don't care" conditions and are not intensified in the 7D01 state table (refer to the Glossary in the General Information section). If there are no differences between state tables, the TABLES= indicator is illuminated.

REF TABLE FOLLOWS 7D01. The FOLLOWS 7D01 mode is functional only when operating in the 7D01 \odot INTENS REF mode. The cursor location (trigger-to-cursor readout) in the reference state table is aligned with the cursor location of the 7D01 state table. As the 7D01 location is changed (by means of the 7D01 cursor position or data position controls), the cursor location of the reference state table follows.

REF TABLE HELD. The HELD mode is functional only when operating in the 7D01 \odot INTENS REF mode. The reference table cursor location remains at one setting, allowing the cursor location in the 7D01 state table to be moved independently (offset). Refer to Figure 2-5.

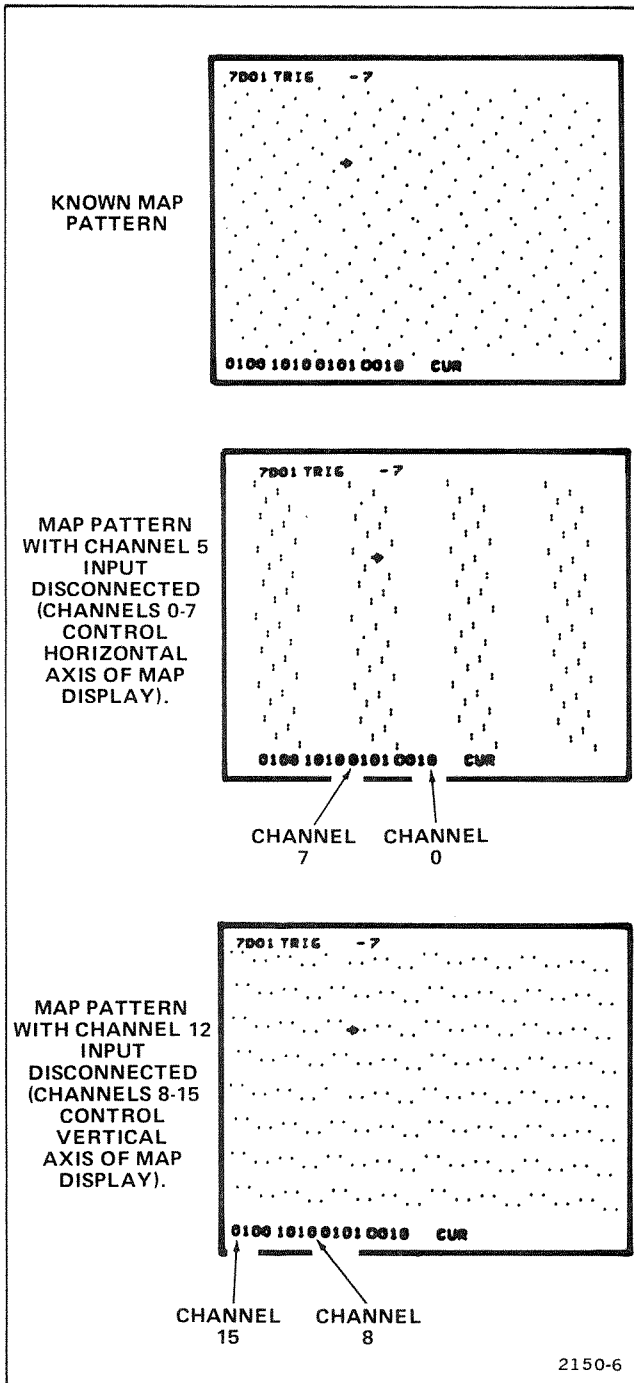


Figure 2-4. Typical map display usage.

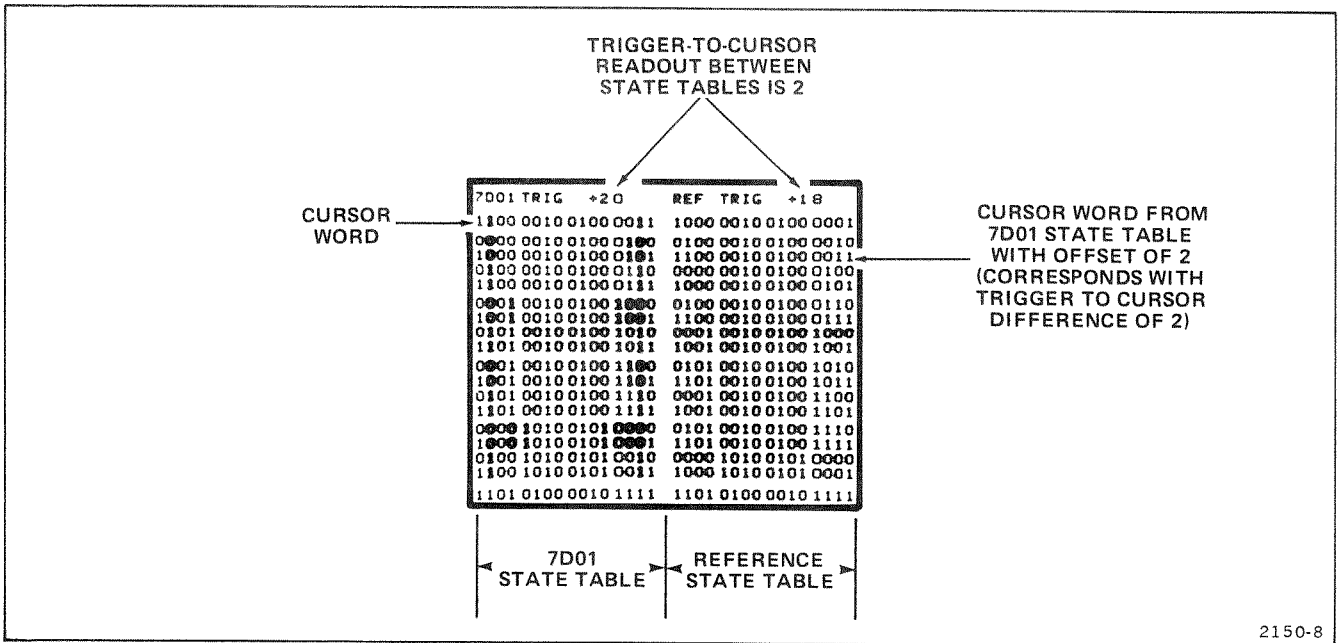


Figure 2-5. Typical state-table display showing offset between the 7D01 and reference state tables.

REF TABLE FOLLOWS WITH/OFFSET. The FOLLOWS WITH/OFFSET mode is functional only when operating in the 7D01 ⊕ INTENS REF mode. The difference in cursor location (offset) between the 7D01 state table and the reference state table, is maintained at the time the FOLLOWS W/OFFSET push button is pressed (see Figure 2-5). The offset between the 7D01 and reference state tables remains constant as the 7D01 cursor is moved. To delete the trigger-to-cursor offset, select REF TABLE FOLLOWS 7D01.

SEARCH. The SEARCH mode is functional when operating in the 7D01 ⊕ INTENS REF mode. When the SEARCH push button is pressed, the 7D01 memory is searched for a match of the reference cursor word. When a match of the reference cursor word is found, the REF TABLE mode is automatically set to HELD and the matching word is moved to the 7D01 cursor word position (first word) of the 7D01 state table.

If a match for the cursor word is not found in the 7D01 memory, the state table display remains unchanged. Also, if the first word in the reference memory is not valid, or a comparison is presently being made in the RESET IF 7D01=REF mode, a search of the 7D01 memory is not made.

RESET IF TABLES=. This mode is functional only when operating in the 7D01 ⊕ INTENS REF mode. When the RESET IF TABLES= push button is pressed, the 7D01

resets and compares the data in the 7D01 state table to the data in the reference state table. If there are no differences, the 7D01 resets, acquires new data, and repeats the comparison. The number of resets is displayed on the crt readout. If there are differences, the acquisition, compare, and reset cycle stops. The differences between state-table displays are intensified in the 7D01 state table. To cancel the RESET IF TABLES= function, a second push of the RESET IF TABLES= push button is required.

RESET IF 7D01=REF. This mode is functional when operating in all DF1 display modes. When the RESET IF 7D01=REF push button is pressed, the data in the 7D01 memory is compared to the data in the reference memory. If there are no differences, the 7D01 resets, acquires new data, and repeats the comparison. The number of resets is displayed on the crt readout. If there are differences, the acquisition, compare, and reset cycle stops. The cursor word is moved to the first difference and the RESET IF 7D01=REF function is canceled. The RESET IF 7D01=REF function may also be canceled with a second push of the RESET IF 7D01=REF push button.

STORE 7D01→REF. This mode is functional in all DF1 display modes (Timing Diagram, Map, and State Table). When the STORE 7D01→REF push button is engaged, the 7D01 memory is transferred into the DF1 reference memory. When the trigger-to-cursor readout is the same in both state table displays, the 7D01 state table is transferred into the reference state table with no intensified bits. However,

if the trigger-to-cursor readout of the state table displays is offset, the 7D01 state table will be transferred to the reference state table with that offset (intensified bits may appear). The tables are equal but offset by the trigger-to-cursor readout (see Figure 2-5). To make the tables equal, either set the 7D01 cursor position controls so that the trigger-to-cursor readout is the same for both state tables or press the REF TABLE FOLLOWS 7D01 push button.

COLUMN BLANKING. Column blanking is functional when operating in any State Table mode. Undesired vertical columns of data can be blanked from the state-table displays (COLUMN BLANK→ push button). The blanked columns are interpreted as "don't care" information for state table comparisons and reset functions (refer to the Glossary in the General Information section). To restore a blanked column, press the COLUMN BLANK← push button. The column blanking function is automatically reset to display or compare all columns when the TIMING DIAGRAM, MAP, STATE TABLE (HEX, OCTAL, BINARY), 7D01 ONLY, or 7D01⊕ INTENS REF push buttons are pressed.

LOGIC STATES. When POS LOGIC is selected, the most positive voltage level is interpreted as a logic HI and the most negative level is interpreted as a logic LO. When NEG LOGIC is selected, the most negative level is displayed as a logic HI and the most positive level is interpreted as a logic LO.

Size and Position Adjustment

The controls used to adjust the size and position of DF1 displays depend on the Display Mode selected.

When operating in the Timing Diagram Display Mode, positioning of the timing diagram display is controlled by

the 7D01 vertical and horizontal position controls. The size of the timing diagram display is determined by the 7D01 vertical and horizontal magnification controls. Vertical positioning of the display readout is controlled by the DF1 front-panel VERT SIZE and VERT POSN adjustments and horizontal positioning is controlled by the DF1 HORIZ POSN adjustment.

When operating in the Map or State Table Display Modes, vertical and horizontal positioning of the entire display (data and readout displays) is controlled by the DF1 front-panel VERT POSN and HORIZ POSN adjustments. Vertical height of the entire display is controlled by the DF1 front-panel VERT SIZE adjustment.

Error Message Displays

Two error messages are provided on the crt readout to identify operator error and instrument failures.

SEE MANUAL CUR CAN'T MOVE. This error message generally occurs when the 7D01 cursor control is set between switch detents. When the error message appears on the crt, move the 7D01 cursor control into a switch detent and the error message should disappear. If the error message does not disappear, refer to the error message discussion in the Maintenance section of the DF1 Instruction Manual.

SEE MANUAL BAD RAM. This error message indicates that a random access memory (RAM) integrated circuit has failed. To test the DF1 for a bad RAM: Turn off power to oscilloscope mainframe, wait a short time, and turn power on (Power-On Mode). Then check the crt readout for an error message. If the error message appears on the crt readout, refer to the error message discussion in the Maintenance section of the DF1 Instruction Manual.

FUNCTIONAL CHECK

The following procedure is provided for familiarization and for checking basic instrument functions of the DF1 Display Formatter. Refer to the Controls and Connectors discussion while performing this procedure. If a malfunction or possible improper adjustment is revealed while performing this procedure, first check the operation of the 7D01 and associated oscilloscope mainframe, then refer to the DF1 Instruction Manual for troubleshooting and adjustment procedures.

The functions are checked without removing the covers or making internal connections. Performance requirements, functions which require removal of side panels, and detailed checks of the DF1 memory are provided in the Performance Check and Adjustment procedures in the DF1 Instruction Manual.

SETUP PROCEDURE

1. Attach the DF1 Display Formatter to the 7D01 Logic Analyzer and install the three-wide plug-in assembly into the oscilloscope mainframe (refer to Installation, in the General Information section, for assembly instructions). Set the oscilloscope mainframe to display the right vertical and A horizontal compartments.

2. Connect the Interface Test Fixture to the 7D01 as shown in Figure 2-6.

3. Set the 7D01 Logic Analyzer controls as follows:

- Sample IntervalExt
- Record Display Time . .∞
- Data PositionPost Trig
- Data Channels0-15
- Trigger SourceW.R.
- Word RecognizerCH 0 through CH 6—LO
CH 7—HI
CH 8 through CH 15—X
External Qualifier—X
Probe Qualifier—X
- W.R. ModeSync
- Threshold Voltage . . .TTL (+1.4 V)

4. Perform the Power-On function (turn mainframe power off, wait a short time, then turn power on).

intensity and the 7D01 vertical and horizontal position/magnification controls.

3. Check that the trigger-to-cursor readout is zero and that the intensified cursor point is superimposed on the intensified trigger point (left-hand side of the crt display).

4. Set the 7D01 Data Position switch to Center and press the Record Manual Reset push button. Check that the trigger point (intensified dots) is near the center of the crt display and that the trigger-to-cursor readout is approximately -112. Rotate the 7D01 Cursor Fine Position control and note that the cursor point (indicated by intensified dots on the left side of the 16-channel display) moves in 1-bit increments as shown by the trigger-to-cursor readout. Rotate the 7D01 Cursor Coarse Position control and note that the cursor point moves in 16-bit increments. Note that the logic state for each channel of displayed data (16-bit readout at bottom of crt) changes corresponding to the cursor position. Set the 7D01 Cursor Position controls for a trigger-to-cursor readout of zero. Check that the intensified cursor point is superimposed on the intensified trigger point (center of crt).

5. Set the 7D01 Data Position switch to Pre Trig and press the Record Manual Reset push button. Check that the trigger point (intensified dots) is at the right-hand side of the display and that the trigger-to-cursor readout is approximately -112. Set the 7D01 Cursor Position controls for a trigger-to-cursor readout of zero. Check that the intensified cursor point is superimposed on the intensified trigger point (right-hand side of crt display).

TIMING DIAGRAM DISPLAY

1. Perform the Setup Procedure.
2. Check crt display for a 16-channel timing diagram (refer to Fig. 2-3). It may be necessary to adjust the mainframe

MAP DISPLAYS

1. Perform the Setup Procedure.
2. Press the MANUAL MAP push button. Check crt display for a diagonal line on the crt (see Fig. 2-7).

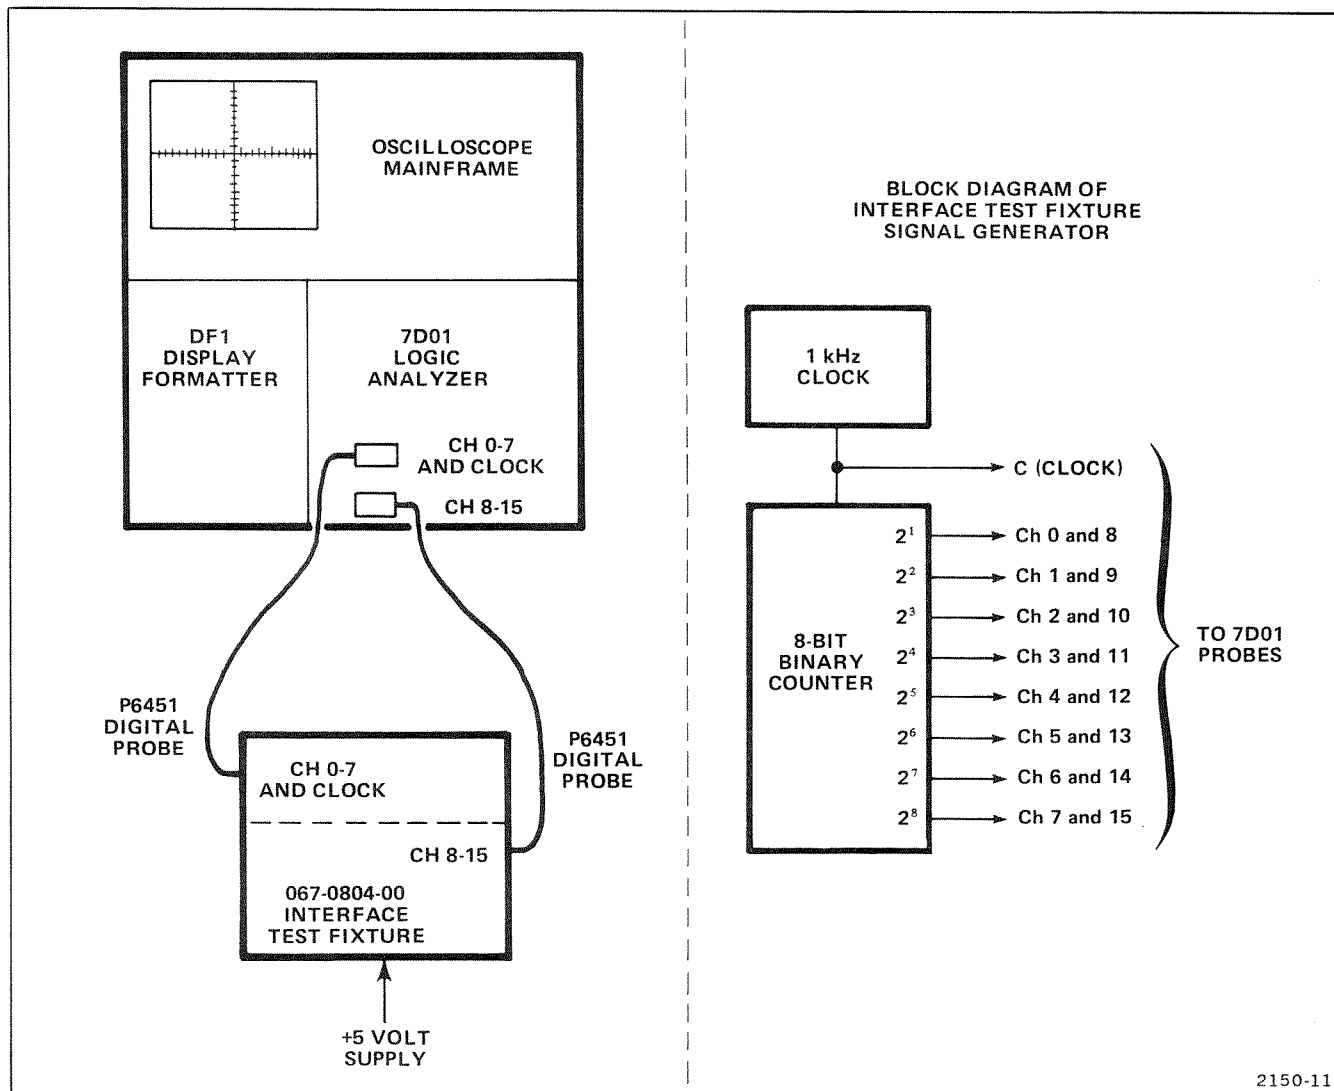


Figure 2-6. Test setup for Functional Check procedure.

3. Rotate the 7D01 Cursor Position controls and note that the cursor point (indicated by a + symbol) can be manually sequenced through the Data as indicated by the trigger-to-cursor readout.

4. Press the SLOW MAP push button and check that the cursor symbol sequences automatically through the data at a slow rate. Press the FAST MAP push button and check that the cursor sequences through the data at a fast rate.

5. Disconnect the channel 5 input from the Interface Test Fixture. Press the 7D01 Record Manual Reset push button and check that the Map display changes to 2 broken diagonal lines (see Fig. 2-8). Reconnect the channel 5 input signal.

STATE TABLE DISPLAYS

1. Perform the Setup Procedure.

2. Press the STATE TABLE HEX push button. Then, press the TIMING DIAGRAM push button and check for 16 channels of data on the crt. Note the logic-state readout of the cursor word, in hexadecimal code, at the bottom of the crt.

3. Press the STATE TABLE HEX and 7D01 ONLY push buttons. Check for a State Table display on left side of the crt in hexadecimal code (base 16). Note that the cursor word (top word in state table) is the same as the cursor word in the Timing Diagram display noted in step 2 and

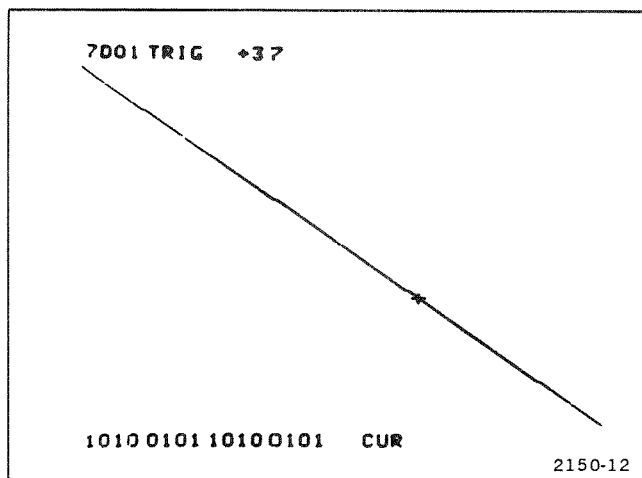


Figure 2-7. Typical map display of 16 channels from the 067-0804-00 Interface Test Fixture.

that the trigger-to-cursor readout is +0. Check that the cursor word is blinking and that the trigger word (bottom) is the same as the cursor word. (Ignore the *'s displayed in the bottom two lines of data.)

4. Rotate the 7D01 Cursor Fine Position control counter-clockwise, 1 bit at a time, until the trigger-to-cursor readout is -16. Check that the blinking word is the seventeenth word in the State Table display.

5. Press the STATE TABLE OCTAL push button. Check that the State Table display is given in the octal (base 8) code.

6. Press the STATE TABLE BINARY push button. Check that the State Table display is given in the binary (base 2) code. Press the NEG LOGIC push button and check that all zeros become ones and that all ones become zeros.

7. Turn off power to the oscilloscope mainframe, wait a short time, and turn power on (Power-On mode). Check crt for Timing Diagram display with trigger-to-cursor readout of zero.

8. Press the STATE TABLE BINARY push button and note the State Table display on the left half of the crt. Press the 7D01 \odot INTENS REF push button and check for a reference state table on the right side of the crt, in addition to the 7D01 state table. Note that the reference state table is all zeros and that the ones in the 7D01 state table are intensified.

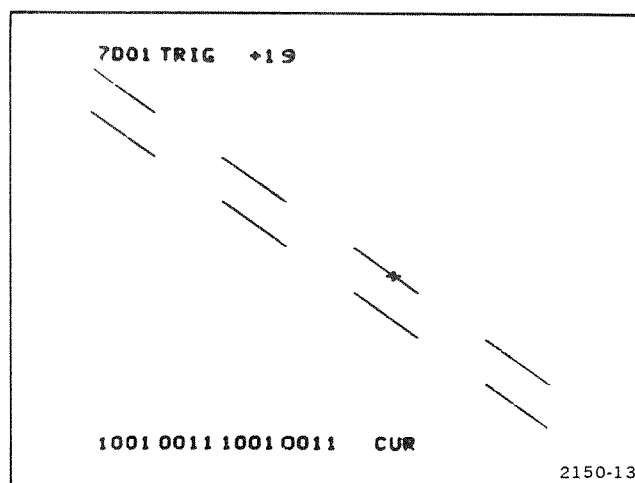


Figure 2-8. Typical map display of 15 channels from the 067-0804-00 Interface Test Fixture (channel 5 input disconnected).

9. Press the SEARCH push button and check that a match of the cursor word in the reference state table (all zeros) is found in the 7D01 memory and transferred to the 7D01 cursor word position (first word in the 7D01 state table). Note that the trigger-to-cursor readout in the 7D01 state table represents the position in memory of the matching word.

10. Set the 7D01 Cursor Position controls for a trigger-to-cursor readout of +0. Press the STORE 7D01 \rightarrow REF push button and check that the 7D01 display is transferred into the reference memory. Note that the trigger-to-cursor readout is +0 for both state tables displayed, and that there are no intensified characters in the 7D01 state table.

11. Press the REF TABLE FOLLOWS 7D01 push button. Rotate the 7D01 Cursor Position controls and check that the trigger-to-cursor readout of the reference state table follows the trigger-to-cursor readout of the 7D01 state table.

12. Press the REF TABLE HELD push button. Rotate the 7D01 Cursor Position controls. Check that the trigger-to-cursor readout in the 7D01 state table changes and the trigger-to-cursor readout in the reference state table remains fixed. Note that intensified bits in the 7D01 state table indicate differences between the displayed state tables.

13. Rotate the 7D01 Cursor Position controls to set the 7D01 trigger-to-cursor readout to +5 and press the REF TABLE FOLLOWS W/OFFSET push button. Rotate the 7D01 Cursor Position controls and check that the

trigger-to-cursor offset between state tables is maintained (offset is obtained in REF TABLE HELD mode).

14. Press the COLUMN BLANK→ push button and check that columns of data are blanked from the State Table displays. The blanked columns are interpreted as "don't care" information for state table comparisons. Press the COLUMN BLANK← push button and check that the blanked columns of data are restored.

15. Press the REF TABLE FOLLOWS 7D01 push button. Check that both state tables have the same trigger-to-cursor readout and that there are no intensified characters in the 7D01 state table. Check that the TABLES= indicator is illuminated.

16. Press the RESET IF TABLES= push button. Check that the state tables are displayed and then reset. The number of resets is displayed below the reference state table. Disconnect channel 0 from the 067-0804-00 Interface Test Fixture. Check that the state tables are not reset and that the number of resets, before the difference, is displayed on the crt. Check that intensified characters in the 7D01 state table are all in the right-hand column (channel 0). Reconnect the channel 0 input to the Interface Test Fixture.

17. Press the RESET IF 7D01=REF push button. Then press the 7D01 Record Manual Reset push button. The 7D01 is reset each time the 7D01 memory and the DF1 reference memory are equal. Check that the number of resets is displayed on the crt readout. Disconnect channel 0 from the 067-0804-00 Interface Test Fixture. Check that both state tables are displayed and that the intensified characters in the 7D01 state table are all in the right-hand column (channel 0). Check that the number of resets, before the difference, is displayed below the reference state table. Reconnect channel 0 to the Interface Test Fixture.

FRONT-PANEL ADJUSTMENTS

1. Perform the Setup Procedure.

2. Rotate the 7D01 Horizontal Position control and note that it horizontally positions the Timing Diagram display. Rotate the 7D01 Horizontal Magnification control and note that it controls the horizontal size of the Timing Diagram display.

3. Rotate the 7D01 Vertical Position control and note that it vertically positions the Timing Diagram display. Rotate the 7D01 Vertical Magnification control and note that it controls the vertical size of the Timing Diagram display.

4. Rotate the DF1 VERT POSN screwdriver adjustment and check that it controls the vertical position of the display readout. Rotate the DF1 VERT SIZE screwdriver adjustment and check that it controls the vertical size of the readout display.

5. Rotate the DF1 HORIZ POSN screwdriver adjustment and check that it horizontally positions the readout display.

6. Rotate the DF1 INTENS CONTRAST screwdriver adjustment and note that it controls the brightness of the readout display.

7. Press the MAP SLOW push button. Rotate the DF1 VERT SIZE screwdriver adjustment and check that it controls the vertical size of the entire Map display. Rotate the DF1 VERT POSN screwdriver adjustment and check that it controls the vertical position of the entire Map display.

8. Rotate the DF1 HORIZ POSN screwdriver adjustment and check that it horizontally positions the entire Map display.

9. Rotate the DF1 INTENS CONTRAST screwdriver adjustment and note that it controls the brightness of the readout display.


10. Press the STATE TABLE BINARY and 7D01 ⊕ INTEN REF push buttons. Rotate the DF1 VERT SIZE screwdriver adjustment and note that it controls the vertical size of the entire State Table display. Rotate the DF1 VERT POSN screwdriver adjustment and note that it vertically positions the entire State Table display.

11. Rotate the DF1 HORIZ POSN screwdriver adjustment and check that it horizontally positions the entire State Table display.

12. Rotate the DF1 INTENS CONTRAST screwdriver adjustment and check that it controls the brightness of the intensified characters in the 7D01 State Table display.

NOTE

The Functional Check procedure is provided for familiarization and for checking basic functions of the DF1 Display Formatter. These functions are checked without removing the covers or making internal connections. Performance requirements, functions which require removal of side panels, and detailed checks of the DF1 memory are provided in the Performance Check and Adjustment procedures in the DF1 Instruction Manual. Only qualified service personnel should perform checks given in the Instruction Manual.

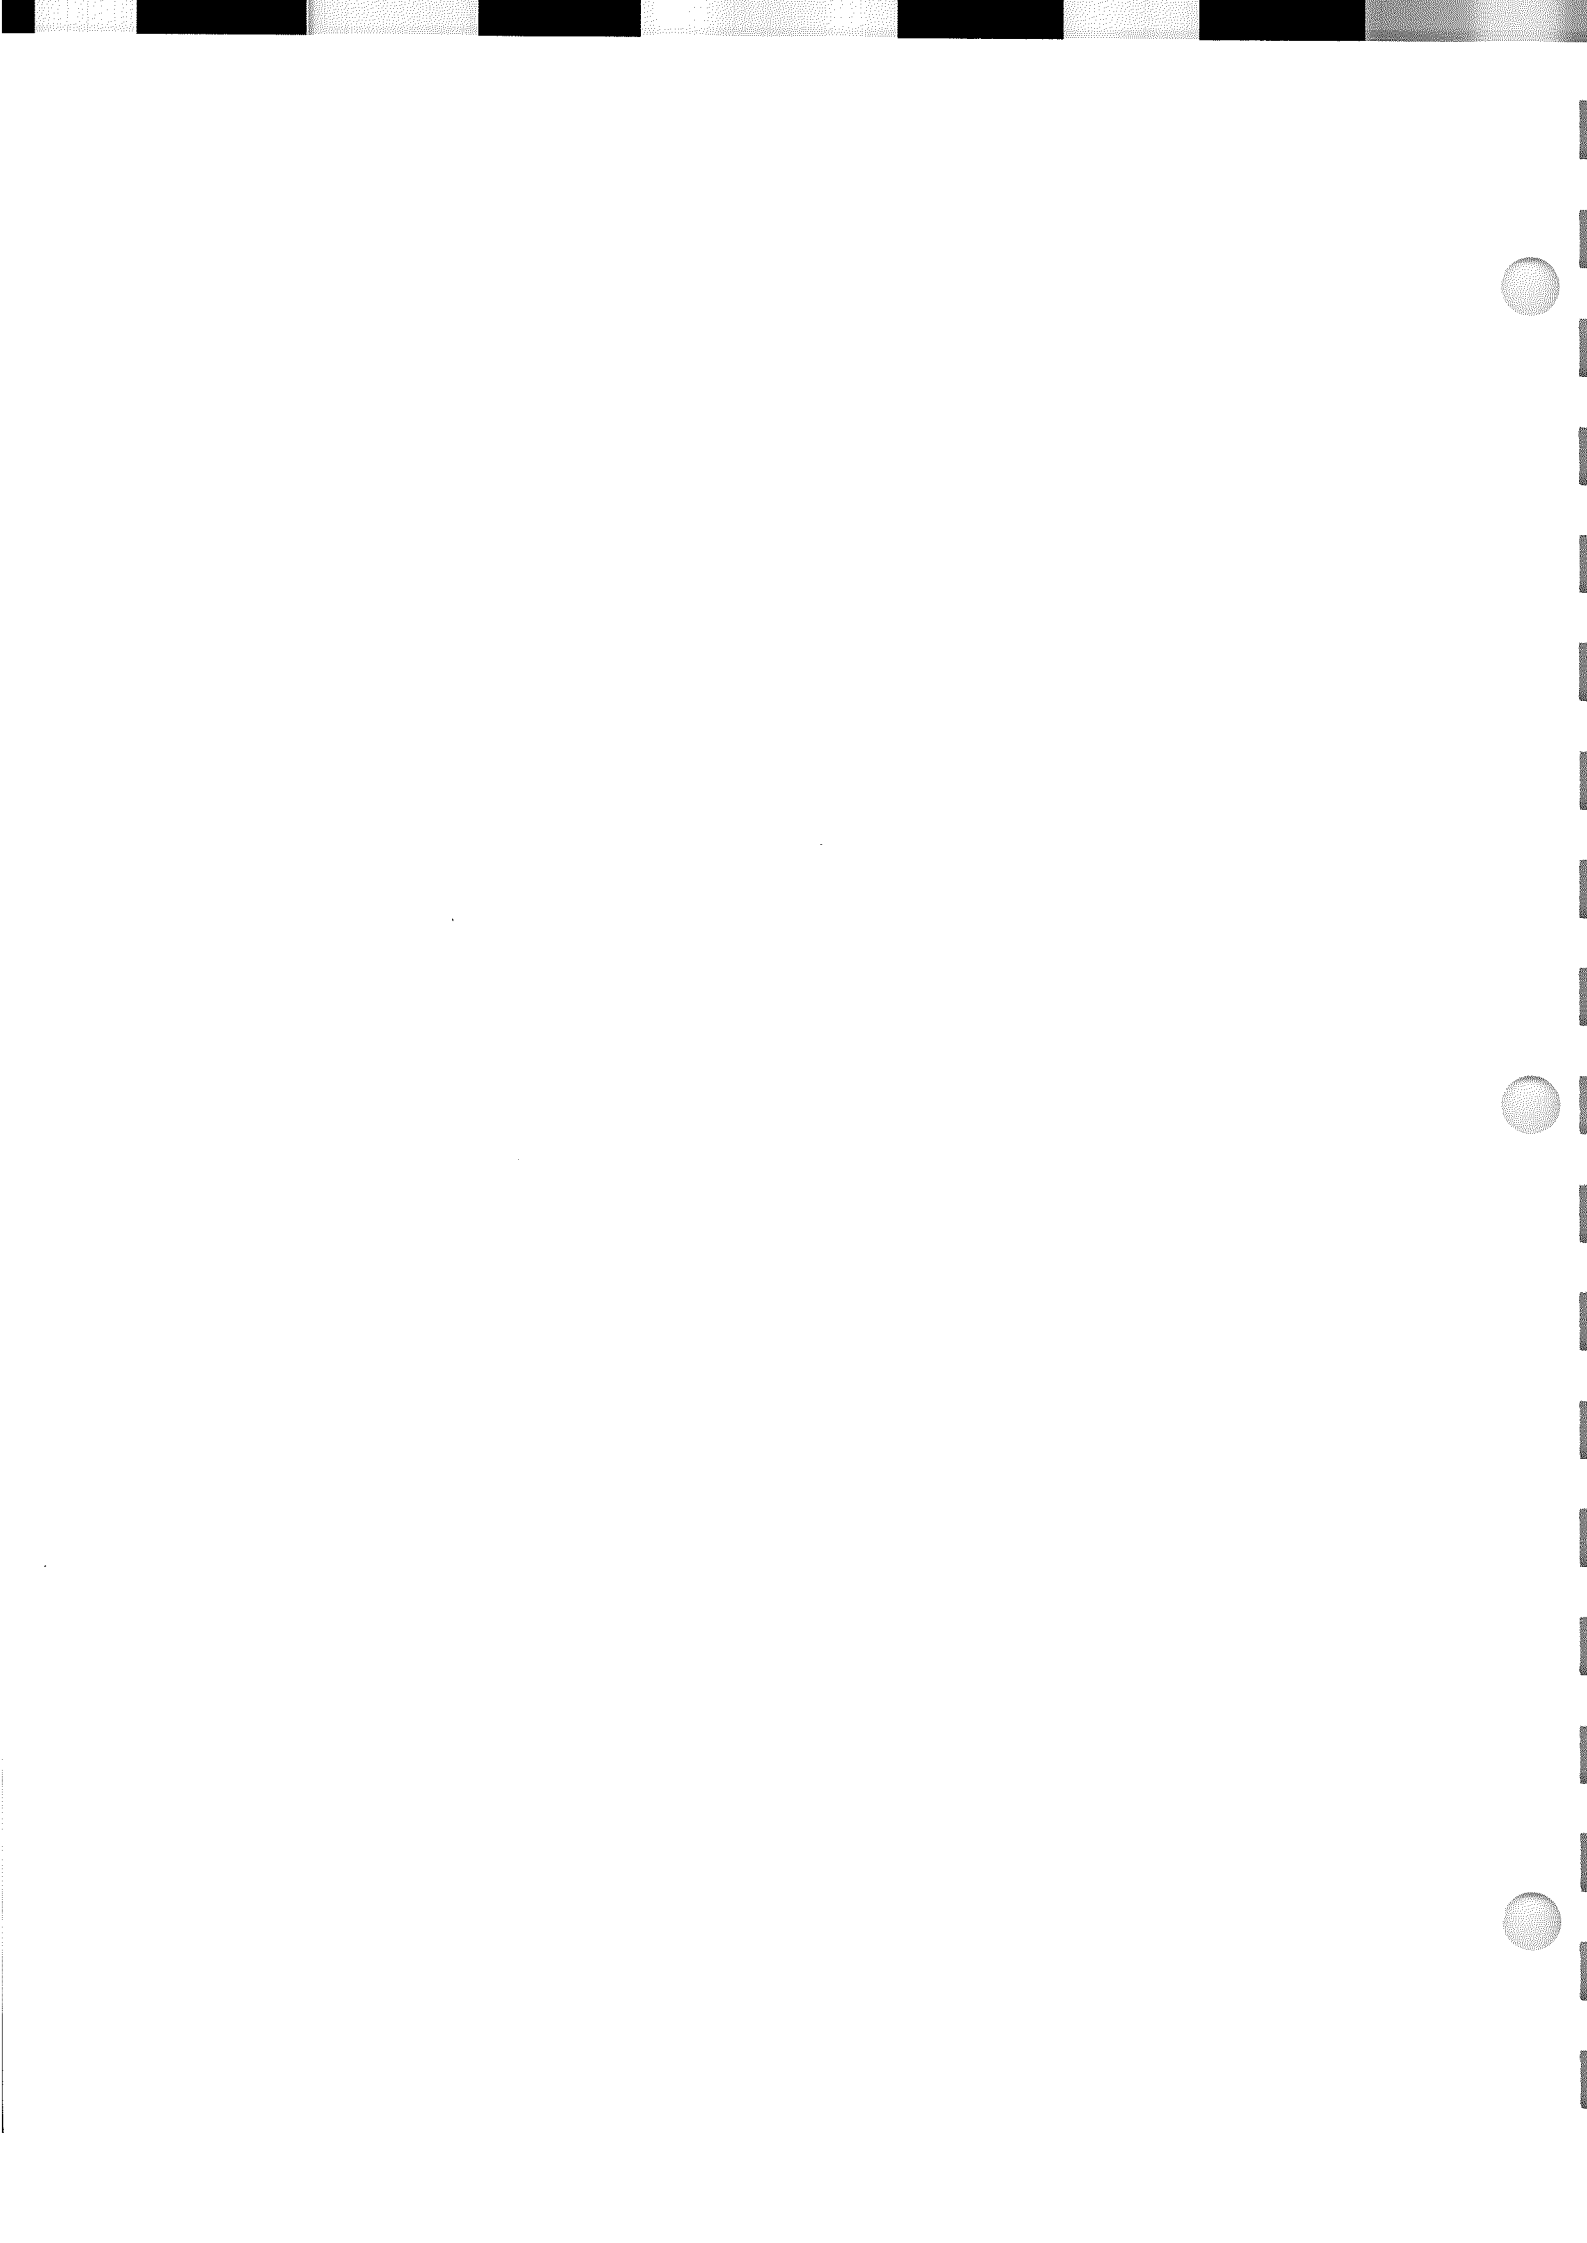

WARNING

THE FOLLOWING SERVICING INSTRUCTIONS ARE FOR USE BY QUALIFIED PERSONNEL ONLY. TO AVOID PERSONAL INJURY, DO NOT PERFORM ANY SERVICING OTHER THAN THAT CONTAINED IN OPERATING INSTRUCTIONS UNLESS YOU ARE QUALIFIED TO DO SO.

THEORY OF OPERATION

The functions of the DF1 are controlled by a microprocessor system built into the instrument. Data and control functions are transferred within the DF1 by an 8-bit data bus and a 16-bit address bus. The microprocessor acquires data from the associated 7D01 Logic Analyzer and performs the functions indicated by the push buttons on the DF1 front panel. The various output displays are coupled back through the 7D01 to the oscilloscope mainframe. Due to the complexity of the DF1 circuitry (especially the microprocessor) normal troubleshooting techniques may not apply to this instrument. See the Maintenance section of this manual for Troubleshooting procedures.

The following descriptions refer to the functional blocks shown on the schematic diagrams in the back of this manual.

FRONT PANEL

The desired function of the DF1 is selected by pressing one of the front-panel switches. When one of the switches is pressed, one of the keyboard lines (KYBD 1 - KYBD 4) drops to a LO level.

The microprocessor must then determine which switch is being pressed. The keyboard line which is being held LO indicates the proper switch column. The row is indicated by clocking a HI level through shift register U65 until the keyboard line returns to a HI level. The shift register is then cleared (all outputs LO). This procedure is repeated five times to eliminate any contact bounce.

EXAMPLE: If the OCTAL button is pressed, KYBD 2 line will go LO. The outputs of U65 are then sequentially driven HI until KYBD 2 goes HI. This occurs on the third clock pulse, identifying the OCTAL switch.

DATA ACQUISITION

The circuitry shown on the Data Acquisition diagram acquires data, cursor, and status information from the 7D01, and connects the keyboard information (KYBD 1 - KYBD 4) to the Data Bus.

Address Decoder

The Address Decoder, U102, provides a single line output for each of eight addresses. Table 3-1 is a truth table for the Data Acquisition Address Decoder.

TABLE 3-1
Data Acquisition Address Decoder

Inputs					Outputs ²
A0	A1	A2	A3	HZP ¹	
LO	LO	LO	LO	LO	$\overline{00B0}$
HI	LO	LO	LO	LO	$\overline{00B1}$
LO	HI	LO	LO	LO	$\overline{00B2}$
HI	LO	HI	LO	LO	$\overline{00B5}$
LO	HI	HI	LO	LO	$\overline{00B6}$
HI	HI	HI	LO	LO	$\overline{00B7}$

¹ Hi Zero Page.

² Outputs change state on rising edge of \emptyset_{2L} signal.

7D01 Cursor Acquisition

The cursor position count is received by the DF1 as ten bits of parallel data. This data is converted to serial data by U132 and U138 and is then clocked through U162 (1D to 1Q) to DB0 (Data Bus line 0).

7D01 Status Acquisition

The operating mode of the 7D01 (store or display) is used by the DF1 to ensure the validity of the acquired data. If the 7D01 goes into store mode while the DF1 is acquiring data, the data acquired would not be valid. The 2Q and 3Q outputs of U162 indicate the status of the 7D01.

Keyboard Latch

The Keyboard Latch, U172, connects the keyboard signal lines (KYBD 1 - KYBD 4) to the data bus (DB4 - DB7).

7D01 Data Acquisition

Data stored by the 7D01 is transferred to the DF1 and stored for faster access by the microprocessor. The data is transferred in serial form and is connected to DB4 (Data Bus line 4) through input 1D and output 1Q of U182.

The frame pulse indicates the beginning of the serial data. When the frame pulse clocks the Q output of U158B LO, the microprocessor starts clocking in the serial data, one bit at a time, by addressing 00B1 to pulse the Display Clock Off line LO for each bit of data.

MPU, PROGRAM, AND DATA STORAGE

This diagram shows the microprocessor, the program ROM (Read Only Memory), and the data-storage and scratch-pad RAMs (Random Access Memories).

Microprocessor

The microprocessor, U264, is the heart of the DF1. All other stages of the circuitry either provide or accept data and/or instructions for (or from) the microprocessor. Due to the complexity of the microprocessor operation, a description of the microprocessor will not be attempted in this manual. If detailed information is needed, refer to the microprocessor manufacturer's specification books.

Program ROM

The Program ROM (Read Only Memory), U284 and U294, provides the permanent storage for the microprocessor instructions. When the microprocessor addresses a location in the Program ROM, the Program ROM connects the addressed information to the Data Bus, which the microprocessor reads and acts on.

Scratch-Pad RAM

The Scratch-Pad RAM (Random Access Memory), U274, provides temporary storage of data or addresses for the microprocessor. The Scratch-Pad RAM can store up to 128 eight-bit bytes of information.

Data Storage RAM

The Data Storage RAM consists of eight RAMs and three Bus Driver integrated circuits. Drivers U304 and half of U308 buffer the address lines to the RAMs. U354 and the other half of U308 provide buffered 3-state outputs for the RAMs to drive the data bus.

VERT AND HORIZ DISPLAY OUTPUT

The Vertical and Horizontal Display Output circuits provide the X-axis and Y-axis deflection for each dot of the State Table or Map displays.

The State Table display consists of 32 columns and 19 rows of characters. Each character contains 5 columns and 7 rows of dots. The State Table display is presented in the following manner: The top row of information (cursor position) is written first. The bottom row of information (trigger word) is written next. The rest of the display is then written, starting with the first row of data and working down. Each row of the display is written from left to right on the crt.

The characters are each written by starting at the top left corner of the character and proceeding across the character to the right edge, then returning to the left edge and dropping to the next row of the character.

The Map display consists of 256 columns and 256 rows of possible dot locations.

Display Column Counter

The Display Column Counter sets the horizontal position of each character of the State Table display. Counter U402 provides the column number (1 to 16) to the ROM, U422. The output of U422 determines the horizontal spacing of the characters. The other 16 columns (columns 17 through 32) are spaced the same as columns 1 through 16, except that they are offset to the right half of the crt display by the HI level at the Q output of U404B. The three-bit or four-bit byte spacing is determined by the level at the E address input of U422. When the E address input is LO, 4-bit byte spacing is provided by the ROM. When the E address line is HI, the other half of the ROM is addressed, providing 3-bit bytes.

Character Column Counter

Character Column Counter U412 provides the horizontal spacing of the five columns of dots for each character. The output of U412 is added to the output of U422 to set the horizontal position of each dot.

Display Row Counter

The Display Row Counter sets the vertical position of each line of the State Table display. Counter U504/U404A provides the row number (1 through 19) to the ROM, U522. The output of U522 determines the vertical spacing of the

rows. Row 1 (cursor location) is written at the top of the crt. Row 2 (trigger word) is written at the bottom of the crt. The other 17 rows are written, in order, starting just below row 1.

Character Row Counter

Character Row Counter U502 provides the vertical spacing of the seven rows of dots for each character. The output of U502 is added to the output of U522 to set the vertical position of each dot.

Display Finish Detector

The Display Finish Detector stops the Display Clock signal after completion of the second or nineteenth display row. The State Table display is finished at completion of row nineteen. The Map and Timing Diagram displays require only the information in rows 1 and 2 (top and bottom). The rest of these displays are provided from other sources.

Character and Dot Position Adders

Adders U432 and U434 combine the outputs of the Display and Character Column Counters to drive the Horizontal D-to-A (digital-to-analog) converter. Adders U552 and U554 combine the outputs of the Display and Character Row Counters to drive the Vertical D-to-A converter.

Map Location Latches

The Map Location Latches accept data directly from the microprocessor, via the Data Bus, to assign dot positions for the Map display. These latches are enabled when the DF1 is in the Map mode.

Map Display Multiplexer

The Map Display Multiplexer selects either State Table or Map display. When the State Table display is selected, the outputs from the adders are coupled through to the Horizontal and Vertical D-to-A converters.

When the Map display is selected, the first two lines (top and bottom) of the State Table are displayed, then the Map Display Multiplexer switches to the Map Location Latch outputs for the remainder of the display.

Vert and Horiz D-to-A Converter

The Digital-to-Analog converters, U468 and U568, each convert eight lines of digital data input to one line of analog data output. The output of each converter is amplified and connected as a push-pull signal to the Vertical or Horizontal outputs to drive the mainframe.

CHARACTER MEMORY AND GENERATOR 5

The Character Memory and Generator circuitry provides the Z-axis (intensity) control for the display.

Next Character Row Counter

The Next Character Row Counter provides the number of the next row of the character being displayed.

Character Latch Decoder

The Character Latch Decoder provides the signals to clock the character address information into U674 and U676.

Next Character Counter

The Next Character Counter provides the address for the next character to be displayed.

RAM Address Switch

The RAM Address Switch allows the Character RAM to be addressed by either the microprocessor (to load the RAM) or by the Next Character Counter (for display).

Character RAM

The Character RAM stores the data required to display each character (as supplied by the microprocessor). The data is then fed to the Present Character Latch one character at a time.

Present Character Latch

The Present Character Latch holds the data from the Character RAM while it is being used. Once this information is latched, the Next Character Counter advances to the address of the next character to be displayed. This "pipeline" effect increases the speed of the display by effectively reducing the access time of the Character RAM to zero.

Present Character Generator and Shift Register

The Present Character Generator, U684, provides five outputs, one for each character column. The five outputs indicate whether the corresponding dots are bright or dark. The five outputs from U684 are loaded into Shift Register U694 and clocked out in sequence to provide the Z-axis (intensity) information for each row of each character.

DISPLAY CONTROL AND Z-AXIS 6

The circuits on this diagram provide the clock and control signals for the display.

65-Hz Clock

The 65-Hz Clock, U640, provides the "refresh" timing for the display.

Blinking Character Counter

The Blinking Character Counter, U648, causes the trigger word to blink when it appears in the State Table display by disabling the z-axis every fourth time the trigger word is displayed.

4-MHz Clock

The 4-MHz Clock provides the display clock signal when gated by the Character Dot Detector. Flip-flop U714A and gate U724D ensure a full-width pulse output for the first enabled clock pulse.

Character Dot Detector

The Character Dot Detector speeds up the display by allowing display time only if a dot is to be displayed. If no dot is to be displayed at the present address, the next pulse from the 4-MHz Clock is coupled to the DSPL CLK line to advance the counters (diagrams 4 and 5) to the next address. If a dot is to be displayed, the Character Dot Detector allows one 4-MHz Clock pulse for the D-to-A converters (diagram 4) to settle, then enables the Z-axis for two 4-MHz Clock pulses before advancing the counters to the next address.

Map Z-Axis

The Map Z-Axis stage enables the z-axis (intensity) for each dot of the Map display. Monostable multivibrator U748A is triggered by the output of U714B to allow the D-to-A converters (diagram 4) to settle. U748B then enables the z-axis to display each dot.

Display Control

The Display Control stage determines the source of the display and readout signals. The readout source is selected by jumper P754. When the jumper is in the MFR (mainframe readout) position, the cursor position and cursor word readout is supplied by the 7D01 in the Timing Diagram mode (the DF1 provides the readout for the other display modes). When the jumper is in the FOR R (formatter readout) position, the DF1 provides the readout for all display modes.

All display information is supplied by the DF1, except for the Timing Diagram display which is provided by the 7D01 directly.

Output Buffers

The Output Buffers provide the final amplification required by the control signals used by the oscilloscope mainframe.

DISPLAY

The Display diagram shows the three shift registers and associated emitter followers and LED's which make up the front-panel lighting for the DF1.

MAINTENANCE

This section of the manual contains information for performing preventive maintenance, troubleshooting, and corrective maintenance.

PREVENTIVE MAINTENANCE

Preventive maintenance consists of cleaning, visual inspection, etc. Preventive maintenance performed on a regular basis may prevent instrument breakdown and will improve the reliability of the instrument. The severity of the environment to which the instrument is subjected determines the frequency of maintenance. A convenient time to perform preventive maintenance is preceding adjustment of the instrument.

CLEANING

The instrument should be cleaned as often as operating conditions require. Accumulation of dirt on components acts as an insulating blanket and prevents efficient heat dissipation which can cause overheating and component breakdown.

CAUTION

Avoid the use of chemical cleaning agents which might damage the plastics used in this instrument. Use a non-residue type of cleaner, preferably isopropyl alcohol, total denatured ethyl alcohol, or TP35. Before using any other type of cleaner, consult your local Tektronix Service Center or representative.

Exterior

Loose dust accumulated on the front panel can be removed with a soft cloth dampened in a mild detergent and water solution. Abrasive cleaners should not be used.

Interior

Dust in the interior of the instrument should be removed occasionally due to its electrical conductivity under high-humidity conditions. The best way to clean the interior is to blow off the accumulated dust with dry, low-pressure air.

Remove any dirt which remains with a soft brush or a cloth dampened with a mild detergent and water solution. A cotton-tipped applicator is useful for cleaning in narrow spaces.

VISUAL INSPECTION

The instrument should be inspected occasionally for such defects as broken connections, improperly seated semi-conductors, damaged circuit boards, and heat-damaged parts.

The corrective procedure for most visible defects is obvious; however, particular care must be taken if heat-damaged components are found. Overheating usually indicates other trouble in the instrument; therefore, it is important that the cause of overheating be corrected to prevent recurrence of the damage.

Switch Contacts

Switch contacts and pads are designed to operate without lubrication for the life of the switch. However, as the switches are not sealed, dust attracted to the contact area may cause the switch contacts to become electrically noisy. Cleaning may be accomplished by flushing the contact area with isopropyl alcohol or kelite (1 part kelite to 20 parts water). Do not use chemical cleaning agents that leave a film or that might damage plastic parts. Do not use cotton swabs or similar applicators to apply cleaning agents, as they tend to snag and leave strands of cotton on the switch contacts. Should it become necessary to remove a switch for replacement or cleaning refer to Component Removal and Replacement in this section.

SEMICONDUCTOR CHECKS

Periodic checks of semiconductors in the instrument are not recommended. The best check of semiconductor performance is actual operation in the instrument. More details on checking semiconductor operation are given under Troubleshooting.

TROUBLESHOOTING

The following information is provided to help you troubleshoot the instrument. Information contained in other sections of the manual should be used along with the following information to aid in locating the defective component. An understanding of the circuit operation is very helpful in locating troubles, particularly where integrated circuits are used.

TROUBLESHOOTING AIDS

Diagrams

Complete schematic diagrams are given on the foldout pages in section 8, Diagrams and Circuit Board Illustrations. The component number and electrical value of each component in this instrument are shown on these diagrams. (See the first page of the Diagrams and Circuit Board Illustrations section for definitions of the reference designators and symbols used to identify components in this instrument.) Important waveforms, and the numbered test points where they were obtained, are located adjacent to each diagram. The portions of circuits mounted on circuit boards are enclosed with heavy, solid-black lines.

Circuit Board Illustrations

To aid in locating circuit boards, a circuit board location illustration appears on the back of the foldout page facing the schematic diagram. In addition, an illustration of the circuit board(s) is included here, with the physical location of the components and waveform test points that appear on the schematic diagram identified. Each circuit board illustration is arranged in a grid locator with an index to facilitate rapid location of components contained in the schematic diagrams.

Troubleshooting Chart

A troubleshooting chart is given in section 8, Diagrams and Circuit Board Illustrations, to aid in locating a defective circuit. Circuit operation is discussed in detail in section 3, Theory of Operation.

Error Messages on Crt

Table 4-1 indicates the action to be taken in the event an error message is displayed on the crt.

TROUBLESHOOTING EQUIPMENT

The following equipment, in addition to that listed in the Performance Check and Adjustment section, is useful for troubleshooting this unit.

System Test Fixture

Description: Effectively replaces microprocessor U264, and allows operator control of the DF1's data bus, address bus, and R/W line. Tektronix Part 067-0746-00.

TABLE 4-1
Error Messages and Responses

Error Message	Action
SEE MANUAL CUR CAN'T MOVE	1. Check that 7D01 cursor position switch (both fine and course) is firmly seated in detent.
	2. Check DF1 and 7D01 cursor circuitry.
	3. Contact your local Tektronix Field Office or representative for factory repair.
SEE MANUAL BAD RAM	1. Check RAMs U314, U316, U318, U320, U334, U336, U338, and U340, or associated circuitry (see Data Bus and RAM Test in this section). Refer to diagram 3 in section 8.
	2. Contact your local Tektronix Field Office or representative for factory repair.

Interface Test Fixture

Description: Serves as a buffer between the System Test Fixture (067-0746-00) and the DF1. Tektronix Part 067-0804-00.

Cable Extender

Description: Allows the DF1 to operate remote from the 7D01 plug-in unit. Tektronix Part 067-0805-00.

Power Supply

Description: Dc voltage supply; voltage +5 volts, within 5%, with a current capability of at least 1 ampere. Recommended TEKTRONIX types: PS501, PS502, or PS505 Power Supplies.

Transistor Tester

Description: Dynamic-type tester. Purpose: Test semi-conductors. Recommended TEKTRONIX types: 576 Curve Tracer, 577/177 Curve Tracer system, 7CT1N Curve Tracer unit and a 7000-series oscilloscope, or a 5CT1N Curve Tracer unit and a 5000-series oscilloscope.

Multimeter

Description: Voltmeter, 10 megohm input impedance and a range from 0 to at least 50 volts dc; accuracy, within 0.1%. Ohmmeter, 0 to 20 megohms. Test probes should be insulated to prevent accidental shorting. Purpose: Check voltage and resistance.

Test Oscilloscope (Storage Type Preferred)

Description: Frequency response, dc to 100 megahertz minimum; vertical deflection factor, 5 millivolts to 5 volts/division. A 10X, 10 megohm voltage probe should be used to reduce circuit loading. Purpose: Check operating waveforms.

Plug-In Extender

Description: Two types of extenders are available. (1) Flexible Plug-In Extender: Tektronix Part 067-0616-00 (two required). (2) Rigid Plug-In Extender: Tektronix Part 067-0589-00 (two required). Purpose: Allows plug-in operation outside the mainframe.

TROUBLESHOOTING TECHNIQUES

Preliminary Troubleshooting Procedure

This preliminary troubleshooting procedure is arranged to check the simple trouble possibilities before proceeding with extensive troubleshooting. The first few checks ensure proper connection, operation, and adjustment. If the

trouble is not located by these checks, the remaining steps aid in locating the defective component. When the defective component is located, it should be replaced using the replacement procedure given under Corrective Maintenance.

1. CHECK CONTROL SETTINGS. Incorrect control settings can indicate a trouble that does not exist. If there is any question about the function or operation of any control, see the Functional Check in the Operating Instructions section of this manual.

2. CHECK ASSOCIATED EQUIPMENT. Before proceeding with troubleshooting, check that the equipment used with this instrument is operating correctly. Check that the signal is properly connected and that interconnecting cables are not defective. Also check the power source. If the trouble persists, this instrument is probably at fault.

3. VISUAL CHECK. Visually check that portion of the instrument in which the trouble is located. Many troubles can be located by visible indications such as unsoldered connections, broken wires, damaged circuit boards, damaged components, etc.

4. CHECK INSTRUMENT ADJUSTMENT. This instrument contains only one adjustment; check the adjustment, or the affected circuit if the trouble appears in one circuit. Complete adjustment instructions are given in the Performance Check and Adjustment section.

5. ISOLATE TROUBLE TO A CIRCUIT. To isolate trouble to a circuit, note the trouble symptom. The symptom often identifies the circuit in which the trouble is located. When trouble symptoms appear in more than one circuit, check the affected circuits by taking voltage and waveform readings. Also check for the correct output signals at the front-panel connector with a test oscilloscope. Incorrect operation of all circuits often indicates trouble in the power supply, microprocessor, ROM's, or bus drivers. Check for correct voltages of the individual supplies. A defective component elsewhere in the instrument can appear as a power-supply trouble and may also affect the operation of other circuits.

6. CHECK VOLTAGES AND WAVEFORMS. Often the defective component can be located by checking for the correct voltage or waveform in the circuit.

7. CHECK INDIVIDUAL COMPONENTS. The following procedures describe methods of checking individual components. Two-lead components that are soldered in place are best checked by first disconnecting one end. This isolates the measurement from the effects of surrounding circuitry.

WARNING

To avoid electric shock, disconnect the power source before removing or replacing semi-conductors.

Transistors. A good check of transistor operation is actual performance under operating conditions. A transistor can be effectively checked by substituting a new component or one that has been checked previously. However, be sure that circuit conditions are not such that a replacement transistor might also be damaged. If substitute transistors are not available, use a dynamic tester. Static-type testers are not recommended, since they do not check operation under simulated operating conditions.

Integrated Circuits. IC's (integrated circuits) can be checked with a voltmeter, test oscilloscope, or by direct substitution. A good understanding of circuit operation is desirable when troubleshooting circuits using IC's. Use care when checking voltages and waveforms around the IC's so that adjacent leads are not shorted together. A convenient means of clipping a test probe to the 14-, 16-, 20-, and 40-pin IC's is with an IC test clip. This device also serves as an extraction tool. The lead configuration for the semiconductors used in this instrument are shown on a pullout page in the front of the diagrams section.

Diodes. A diode can be checked for an open or shorted condition by measuring the resistance between terminals with an ohmmeter. Use a scale having a low internal source current, such as the R X 1 kΩ scale. The resistance should be very high in one direction and very low when the meter leads are reversed.

CAUTION

Do not use the ohmmeter on a scale that has high internal current. High currents may damage the diode.

The cathode end of each glass-encased diode is indicated by a stripe, a series of stripes, or a dot. The cathode and anode ends of metal-encased diodes are identified by the diode symbol marked on the case.

Resistors. Check resistors with an ohmmeter. See the Replaceable Electrical Parts list for the tolerance of the resistors used in this instrument. Resistors normally do not need to be replaced unless the measured value varies widely from that specified.

Inductors. Check for open inductors by checking continuity with an ohmmeter. Shorted or partially shorted inductors can usually be found by checking the waveform response when high-frequency signals are passed through the circuit. Partial shorting often reduces high-frequency response (roll off).

Capacitors. A leaky or shorted capacitor can usually be detected by checking resistance with an ohmmeter set on its highest scale. Do not exceed the voltage rating of the capacitor. The resistance reading should be high after the initial charge of the capacitor. An open capacitor can best be detected with a capacitance meter or by checking if the capacitor passes ac signals.

8. REPAIR AND ADJUST. If any defective parts are located, follow the replacement procedures given in Corrective Maintenance. Be sure to check the performance of any circuit that has been repaired or had any electrical components replaced.

Troubleshooting with the System Test Fixture

Index to troubleshooting the DF1 with the 067-0746-00 System Test Fixture.

	PAGE
Preliminary Setup Information	4-4
Data Bus and RAM Test	4-6
ROM Test	4-6
Keyboard Test	4-7
Button Lights Test.	4-8
Display Test	4-8
7D01 Control Signals	4-10
7D01 Acquisition	4-11
Reset Output	4-13

PRELIMINARY SETUP INFORMATION. Perform the following steps before proceeding to any of the individual procedures.

- a. Connect test equipment as shown in Figure 4-1. The Interface Test Fixture is connected to the DF1 Intelligence circuit board as shown in Figure 4-2.
- b. Set the System Test Fixture (067-0746-00) control switches (LATCH, FIXTURE, BREAK, INSTR CYCLE) to the Off position.

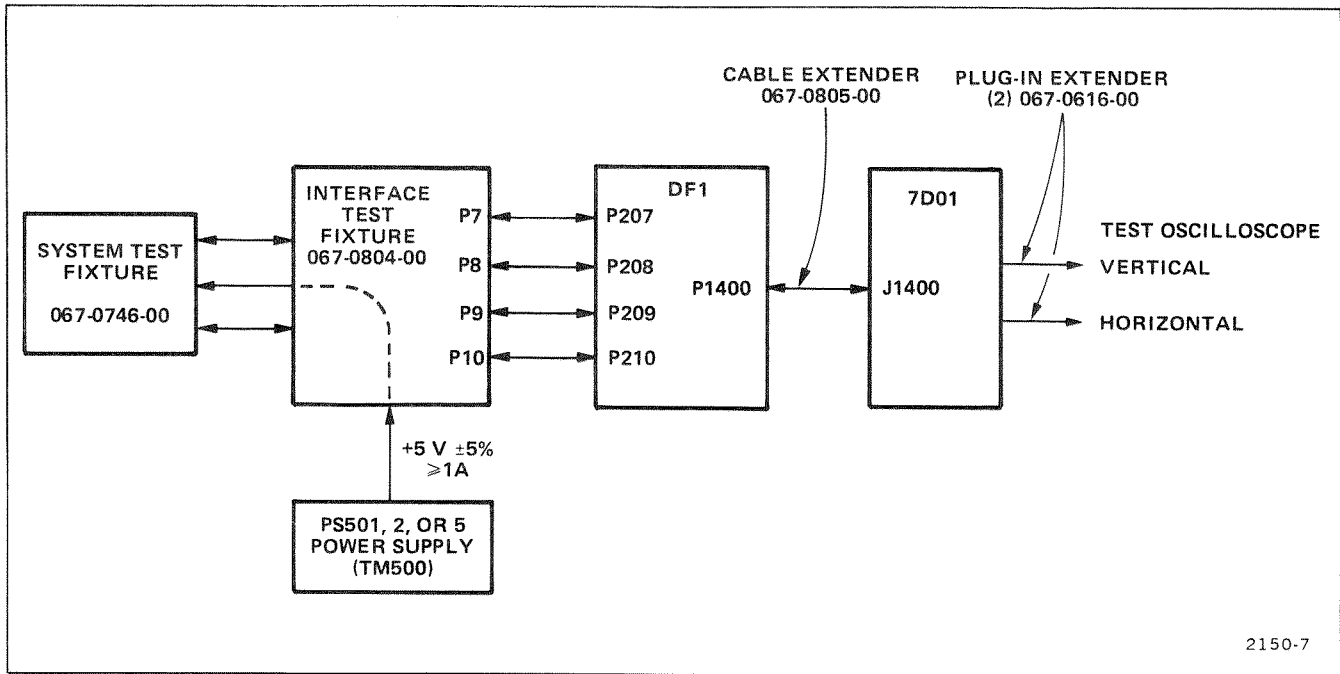


Figure 4-1. Test equipment setup for troubleshooting the DF1 Digital Formatter.

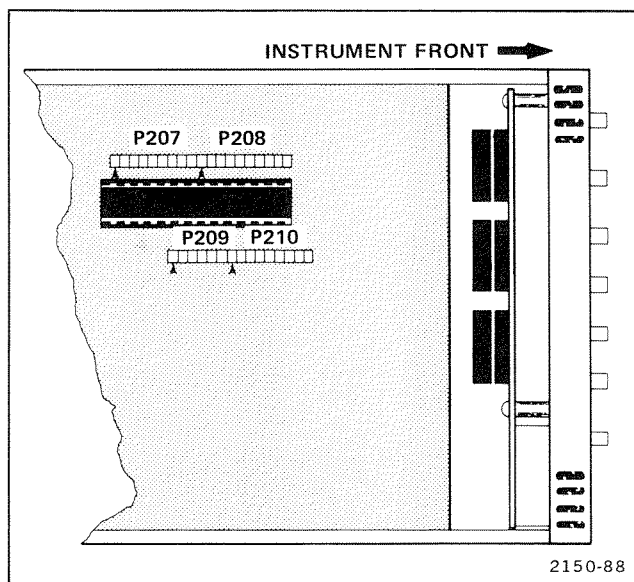


Figure 4-2. Partial view of Intelligence circuit board. Shows pin location and indexing for connection to the Interface Test Fixture.

c. Press the STOP button; the ABA (address bus available) indicator should light. If the ABA indicator does not light, press the RESTART button. If the ABA indicator still does not light, recheck the test equipment setup illustrated in Figure 4-1. Also, check the DF1 clock circuits (O1, O2), reset circuit, power supplies, and the Halt line (pin 2 of U264). Check that the BA output (pin 7 of U264) is not excessively loaded or shorted (low). If the ABA indicator

does not light, and all the above functions operate properly, either the test fixture or U264 is defective.

d. Once the ABA indicator is on, the 067-0746-00 System Test Fixture is effectively replacing the DF1 micro-processor (U264).

NOTE

The System Test Fixture DATA and ADDRESS switches, and the EXAMINE and DEPOSIT push buttons control the DF1's data bus, address bus, and R/W line. At all times during this troubleshooting procedure, disregard the condition of the Address lights on the System Test Fixture.

e. All references to the setting of the ADDRESS and DATA switches will be in base 16 (hexadecimal) to indicate how each group of 4 switches is set, or each group of 4 lights is read. Refer to Table 4-2 for Hex-to-Binary conversion.

f. In general, if a peripheral does not operate properly on a Deposit or Examine function of one of its addresses, the line that generates that address should be checked (with a logic analyzer or a storage scope) to determine if it is pulsed low. If the line is not pulsed low, the defect will be in either the address coding circuitry or the System Test Fixture.

TABLE 4-2
Hex-to-Binary Conversion

Hex	Binary	Hex	Binary
0	0000	8	1000
1	0001	9	1001
2	0010	A	1010
3	0011	B	1011
4	0100	C	1100
5	0101	D	1101
6	0110	E	1110
7	0111	F	1111

DATA BUS AND RAM TEST. The object of this test is to ensure that the data bus lines are independent of each other, and no other peripheral is controlling the bus.

NOTE

A complete cell-by-cell test of only the Data RAM is executed by the DF1 microprocessor upon Restart. A defective cell is indicated on the crt display as "SEE MANUAL BAD RAM".

The testing method used is to address a RAM cell, write into it (Deposit), then read it (Examine). This is accomplished as follows:

- a. Set the System Test Fixture (ADDRESS switches) to correspond to an address in one of the following RAM's.
 1. Scratch pad RAM (Hex addresses 0000 through 007F).
 2. Data RAM (Hex addresses 6000 through 63FF).

EXAMPLE:

The Scratch pad RAM, Hex address 007F, converted to binary is — 0000 0000 0111 1111. Select the ADDRESS switches on the System Test Fixture to match this address.

- b. Set all (except one) of the System Test Fixture DATA switches to 0.
- c. Press the DEPOSIT button, then the EXAMINE button, and note how the Data lights compare with the switches. The information you have put in the DATA switches

should match the Data lights. Continue testing the data buses with a different switch high (1) each time. If, at any point the lights don't agree with the switch positions, check the RAM addressing and support circuits.

- d. Set all (except one) of the System Test Fixtures DATA switches to 1. Repeat step c with a different switch set low (0) each time.

NOTE

If at any time the Data lights do not match the DATA switches in steps c and d, the problem is either a bad RAM IC, some other IC on the bus not being disabled, or the buses are either shorted together, to ground, open, or tied to Vcc. A good method to isolate an IC, which is not getting off the bus, is to disconnect the IC's on the data bus, one at a time, until the problem disappears.

ROM TEST. The object of this test is to ensure that the ROM IC's (U284, U294) are being addressed, and that they drive the data bus.

The method is to read (Examine) several addresses in each of the above ROM's and check that the proper output appears on the System Test Fixture Data lights. This is accomplished as follows:

- a. Set the System Test Fixture (ADDRESS switches) to correspond to an address of one of the ROM IC's shown in Table 4-3.

EXAMPLE: ROM U284

Hex address F800 converted to binary is — 1111 1000 0000 0000 (refer to Table 4-2). Select the ADDRESS switches on the System Test Fixture to match this address.

- b. Press the System Test Fixture EXAMINE button, and note how the Data lights compare with the Data Output listed for that address in Table 4-3.
- c. If the Data lights do not match the Data Output listed, the address pins of the IC in question should be checked with a storage type test oscilloscope, or a logic analyzer to determine if:
 1. The IC is being enabled (chip selects are correct).
 2. The address lines A0-A10 levels correspond to the ADDRESS switch.

TABLE 4-3
ROM Hexadecimal Output Program

ROM U284		ROM U294	
Address	Data Output	Address	Data Output
F800	38	F000	CE
F801	39	F001	00
F802	8D	F002	00
F804	86	F004	00
F808	26	F008	7F
F810	10	F010	55
F820	39	F020	26
F840	97	F040	25
F880	F0	F080	C1
F900	13	F100	DF
FA00	73	F200	97
FC00	84	F400	5C

If the IC in question passes these last two checks (and the DF1 passed the previous test, Data Bus and RAM Test), substitute the IC with a known good ROM.

KEYBOARD TEST. The object of this test is to check for proper operation of the Keyboard circuit.

NOTE

A failure could originate in the Keyboard circuit IC's (U65, U172), the address decoding for them, or the interconnections on one of the specific push buttons used in the test.

If a specific push button switch appears to malfunction, first review the Detailed Operating Instructions (in section 2 of this manual). This will confirm the normal operation for that switch in a particular mode. If the malfunction persists, and the problem is not a defective switch or dirty contacts, proceed to the Keyboard Circuit Checkout Procedure in Table 4-4.

TABLE 4-4
Keyboard Circuit Checkout Procedure

Step	System Test Fixture		Comment
	Address	Data Light Display ¹	
1	00B6	XX ²	Clears U65.
2	Hold down TIMING DIAGRAM button on DF1.		
3	00B0	EX ²	Reads a Kybd 1 key down. ³
4	00B0	FX ²	Reads TIMING DIAGRAM key.
5	Hold down OCTAL button on DF1.		
6	00B0	DX ²	Reads a Kybd 2 key down. ³
7	00B0	FX ²	Reads OCTAL key down.
8	Hold down COL BLANK← button on DF1.		
9	00B0	BX ²	Reads Kybd 3 key down. ³
10	00B0	FX ²	Reads ← down.
11	Hold down STORE 7D01→ REF button on DF1.		
12	00B0	7X ²	Reads Kybd 4 key down. ³
13	00B0	FX ²	Reads STORE key down.

¹ The X means "disregard the lights in that part of the display".

² Press the System Test Fixture EXAMINE button.

³ Refer to diagram 1 in the Diagrams and Circuit Board Illustrations section.

BUTTON LIGHTS TEST. The object of this test is to assure that each of the DF1 button lights operate properly.

NOTE

The DF1 SEARCH and STORE 7D01→REF buttons do not have lights.

The button lights in the DF1 are driven by the outputs of a serial-to-parallel shift register. The System Test Fixture data bus 7 (DATA switch number 7) is the input, and a press of the DEPOSIT button (address 00B2) is the clock of this shift register.

Table 4-5 lists the number of times the DEPOSIT button must be pushed in order to control a given DF1 button light.

TABLE 4-5
Manual Clock Pulses Required To Control Button Lights

Number of Deposits (Clock)	Button Light
1	TIMING DIAGRAM
2	FAST
3	SLOW
4	MANUAL
5	Not Used
6	HEX
7	OCTAL
8	BINARY
9	Not Used
10	7D01 ONLY
11	⊕ INTENS REF
12	TABLES= (Indicator light)
13	POS
14	NEG
15	←
16	→
17	FOLLOWS 7D01
18	HELD
19	FOLLOWS W/OFFSET
20	Not Used
21	7D01=REF
22	TABLES= (button light)

To completely check the button lights, proceed as follows:

- a. Set the System Test Fixture DATA switch number 7 HI (1), and the ADDRESS switches for 00B2 (refer to Table 4-2).
- b. Press the System Test Fixture DEPOSIT (manual clock) button the required number of times shown in Table 4-5, and note that the specified button light comes on.
- c. Set the System Test Fixture DATA switch number 7 LO (0).
- d. Repeat step b and note the button light goes off.
- e. Repeat steps a through d for each of the button lights listed in Table 4-5.

If a button light fails to either turn on or off, check the LED, associated transistor, shift register, or the LED power supply (VR62, CR62, and R62).

DISPLAY TEST. There are four control bits with which the microprocessor controls the display. Two of these are at address 00A8. The other two (at address 0098) are used to control operation when in the 7D01 Timing Diagram mode. Checkout for proper display function is accomplished as follows:

- a. Connect the DF1 Readout Source multi-pin jumper (internal) to display the formatter readout (FOR R). Refer to Figure 4-3.
- b. Set the System Test Fixture ADDRESS switches to 00A8, and the DATA switches as shown for that address on line 1 of Table 4-6.
- c. Press the DEPOSIT button.
- d. Set the System Test Fixture ADDRESS switches to 0098, and the DATA switches as shown for that address on line 1 in Table 4-6.
- e. Press the DEPOSIT button.

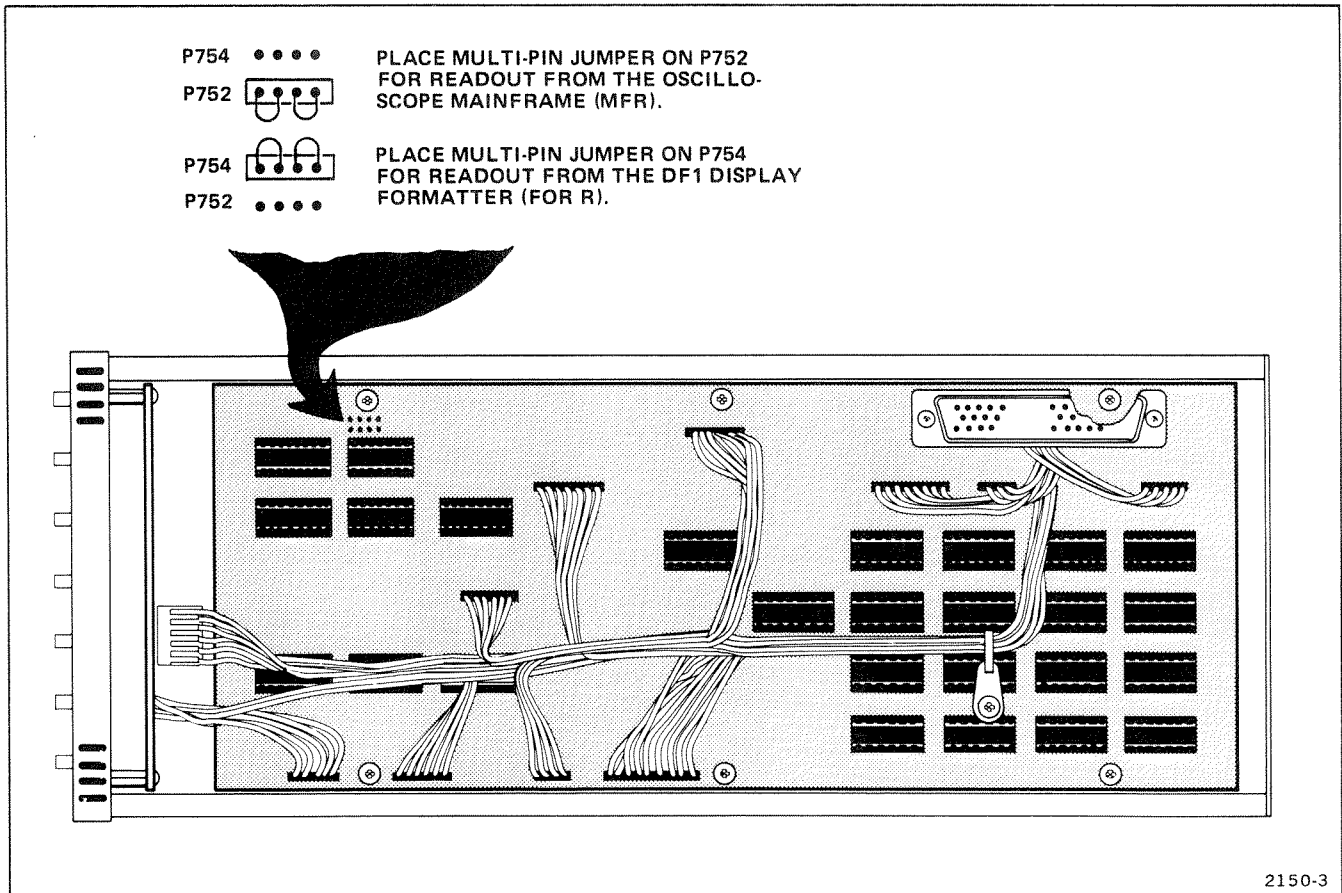


Figure 4-3. Location of readout source multi-pin jumper.

TABLE 4-6
Formatter Readout Truth Table

Line #	Data Switch Number				Display	
	(Address 00A8)		(Address 0098)			
	3*	1	0	3	0*	
1	X	0	0	1	X	Map mode, with 2 lines of DF1 readout. (No map is visible.)
2	1	1	0	1	1	Display 7D01 with 2 lines of DF1 readout, if triggered. ¹
3	1	1	0	0	1	Display 7D01 only—no DF1 readout, if triggered. ¹
4	X	0	1	X	X	Not a valid display.
5	X	1	1	X	X	Displays 19 lines of DF1 readout.

1 = HI, 0 = LO, X = DON'T CARE

*Control signals necessary only to produce a Timing Diagram display.

¹ If the 7D01 is not triggered, verify performance of the 7D01; check DF1's "7D01 reset" circuit; check that 7D01 sample interval switch is not in the external position.

Maintenance—DF1

f. Check for the proper display (as shown in Table 4-6 for line 1). If the display is correct, repeat the above procedure for lines 2, 3, 4, and 5 of Table 4-6.

g. Connect the DF1 Readout Source multi-pin jumper (internal) to display mainframe readout (MFR). Refer to Figure 4-3.

h. Repeat steps b through f, using Table 4-7.

NOTE

If the display does not match that shown in Tables 4-6 and 4-7, first check the mode decoding circuitry, then the display. HINT—If the display doesn't work, follow the counter clocks around to assure they are all operating.

7D01 CONTROL SIGNALS. There are three control lines with which the microprocessor can directly control the 7D01.

Set up conditions as follows:

a. Connect the DF1 Readout Source multi-pin jumper (internal) to display the mainframe readout (MFR). Refer to Figure 4-3.

b. Set the System Test Fixture ADDRESS switches to 0098, and DATA switch number 0 to HI (1).

c. Press the DEPOSIT button.

d. Set the System Test Fixture ADDRESS switches to 00A8. Set DATA switches: number 3 to HI (1), number 1 to HI (1), and number 0 to LO (0).

e. Press the DEPOSIT button.

f. Press the 7D01 manual trigger button.

1. Cursor Increment. Check as follows:

a. Set the System Test Fixture ADDRESS switches for 00B7.

b. Press the EXAMINE button and observe that the cursor display on the crt moves one increment. Check that the cursor moves one increment each time the EXAMINE button is pressed.

NOTE

If the cursor does not perform properly, check that the 7D01 cursor position switch (both course and fine) are firmly seated in a detent; also check the cursor clock circuitry.

2. Display Clock. Check as follows:

TABLE 4-7

Mainframe Readout Truth Table

Line #	Data Switch Number			Display
	(Address 00A8) 3* 1 0	(Address 0098) 0		
1	X 0 0	0		Map mode, except for 2 lines DF1 readout.
2	X 1 0	0		No 7D01 display or readout.
3	1 1 0	1		Display 7D01 only, with readout, if triggered. ¹
4	X 0 1	X		Not a valid display.
5	X 1 1	0		Displays 19 lines of DF1 readout.

1 = HI, 0 = LO, X = DON'T CARE

*Control signals necessary only to produce a Timing Diagram display.

¹ If the 7D01 is not triggered, verify performance of the 7D01; check DF1's "7D01 reset" circuit; check that 7D01 sample interval switch is not in the external position.

- a. Set the System Test Fixture ADDRESS switches to 0098. Set DATA switch number 0 to LO (0).
- b. Press the DEPOSIT button. The crt display should disappear.
- c. Set the System Test Fixture DATA switch number 0 to HI (1).
- d. Press the DEPOSIT button. The crt display should return.

NOTE

Address 0098 determines if the 7D01 display clock is on or off.

3. 7D01 Reset. Check as follows:

- a. Set the System Test Fixture ADDRESS switches to 00A8. Set DATA switches: number 1 to HI (1), number 0 to LO (0), and number 3 to LO (0).
- b. Press the DEPOSIT button. The 7D01 trig'd light should go out, and the crt display should disappear.
- c. Set the System Test Fixture DATA switch number 3 to HI (1).
- d. Press the DEPOSIT button.
- e. Press the 7D01 manual trigger button. The crt display should return, and the trig'd light should stay on.

NOTE

DATA switch number 3 at address 00A8 controls the 7D01 reset.

7D01 ACQUISITION. Since the DF1's acquisition of the 7D01's data is handled entirely by the microprocessor, this is the most complex interface. Check the Acquiring states of cursor counters, Acquiring 7D01 status, and Acquiring contents of 7D01 memory, as outlined in the following procedures.

Set up conditions as follows:

@

- a. Connect the DF1 Readout Source multi-pin jumper (internal) to display the mainframe readout (MFR). Refer to Figure 4-3.
- b. Set the System Test Fixture ADDRESS switches to 0098, and DATA switch number 0 to HI (1).
- c. Press the DEPOSIT button.
- d. Set the System Test Fixture ADDRESS switches to 00A8. Set the DATA switches: number 3 to HI (1), number 1 to HI (1), and number 0 to LO (0).
- e. Press the DEPOSIT button.
- f. Press the 7D01 manual trigger button.

1. CURSOR ACQUISITION. Check as follows:

- a. Set the 7D01 data channels switch to 0-15.
- b. Rotate the 7D01 cursor position switch (fine and course) to position the intensified dot one click before it disappears from the right side of the crt display.
- c. Set the System Test Fixture ADDRESS switches to 00B6.
- d. Press the EXAMINE button.
- e. Set the System Test Fixture ADDRESS switches to 00B0.
- f. Press the EXAMINE button 8 times, and observe that the Data light number 0 stays off.
- g. Press the EXAMINE button 6 times. Data light number 0 should turn on.
- h. Press the EXAMINE button once, and observe that Data light number 0 turns off.
- i. Press the EXAMINE button once, and observe that Data light number 0 turns on again.

Maintenance—DF1

- j. Rotate the 7D01 cursor position switch (fine) one click (dot disappears from the display).
- k. Set the System Test Fixture ADDRESS switches to 00B6.
- l. Press the EXAMINE button.
- m. Set the System Test Fixture ADDRESS switches to 00B0.
- n. Press the Examine button exactly 14 times. The Data bus light number 0 should remain lit through all 14 Examines.
- o. Press the EXAMINE button 2 more times. The Data light number 0 should be off both times.

2. 7D01 STATUS. Check as follows:

NOTE

The 7D01 should be in external trigger, with no input.


- a. Press the 7D01 manual reset button.
- b. Set the System Test Fixture ADDRESS switches to 00B0.
- c. Press the EXAMINE button.
- d. Check that Data light number 2 is off.
- e. Press the 7D01 manual trigger button.
- f. Press the EXAMINE button. Observe that Data light number 2 is on.
- g. Set the System Test Fixture ADDRESS switches to 00B5.
- h. Press the EXAMINE button.

- i. Set the System Test Fixture ADDRESS switches to 00B0.
- j. Press the EXAMINE button. Observe that Data light number 1 is off.
- k. Press the 7D01 manual reset button.
- l. Press the 7D01 manual trigger button.
- m. Press the EXAMINE button. Observe that Data light number 1 is on.

3. 7D01 Memory. Check as follows:

- a. Connect the two P6451 probes (7D01 standard accessories) to the 7D01 connectors.

- b. Set the 7D01 front-panel controls as follows:

Threshold VoltageTTL
 Sample IntervalExternal
 Ext Clock Polarity
 Data Channels0-15
 Data PositionPost Trig

- c. Connect the P6451 probe test leads as follows:
 - (1) Both probe ground leads to the Interface Test Fixture ground terminals.
 - (2) Channel 12 probe lead to terminal 0.
 - (3) External clock probe lead to terminal C.
- d. Press the 7D01 manual reset button.
- e. Press the 7D01 manual trigger button (if trig'd light is not on).
- f. Set the System Test Fixture ADDRESS switches to 0098. Set DATA switches: number 3 to HI (1), and number 0 to LO (0).
- g. Press the DEPOSIT button.

NOTE

If a bright dot appears on the crt display, either position it off-screen, or reduce the oscilloscope intensity.

- h. Set the System Test Fixture ADDRESS switches to 00B1.
- i. Press the EXAMINE button.
- j. Check that Data light number 5 is on, number 6 is on, and number 7 is off.
- k. Press the EXAMINE button once. Data light number 4 should change state.
- l. Press the EXAMINE button once. Data light number 5 should go off, and Data light number 4 should change state again.
- m. Continually press the EXAMINE button. Note that Data light number 5 remains off, light number 6 remains on, and light number 4 changes state with each press of EXAMINE. Stop pressing the EXAMINE button when Data light number 7 comes on (approximately 15-20 Examines).
- n. Press the EXAMINE button once more. Check that Data light number 7 is off, and that light number 4 changes state.

RESET OUTPUT. The logic level of the DF1 reset output (RESET OUT jack on DF1 front panel) is the inverse of whatever is deposited into the System Test Fixture DATA switch 1 at address 0098.

CORRECTIVE MAINTENANCE

Corrective maintenance consists of component replacement and instrument repair. Special techniques required to replace components in this instrument are given here.

OBTAINING REPLACEMENT PARTS

All electrical and mechanical part replacements can be obtained through your Tektronix Field Office or representative. However, many of the standard electronic components can be obtained locally in less time than is required to order them from Tektronix, Inc. Before purchasing or ordering replacement parts, check the parts list for value, tolerance, rating, and description.

NOTE

When selecting replacement parts, it is important to remember that the physical size and shape of a component may affect its performance in the instrument, particularly at high frequencies. All parts should be direct replacements unless it is known that a different component will not adversely affect instrument performance.

Some parts are manufactured or selected by Tektronix, Inc. to satisfy particular requirements, or are manufactured for Tektronix, Inc. to our specifications. Most of the mechanical parts used in this instrument have been manufactured by Tektronix, Inc. To determine the manufacturer of parts, refer to parts list, Cross Index Mfg. Code Number to Manufacturer.

When ordering replacement parts from Tektronix, Inc., include the following information:

1. Instrument type.
2. Instrument serial number.
3. A description of the part (if electrical, include circuit number).
4. Tektronix part number.

WARNING

To avoid electric shock, disconnect the instrument from the power source before soldering.

SOLDERING TECHNIQUES

The reliability and accuracy of this instrument can be maintained only if proper soldering techniques are used when repairing or replacing parts. General soldering techniques, which apply to maintenance of any precision electronic equipment, should be used when working on this instrument. Use only 60/40 rosin-core electronic-grade solder. The choice of soldering iron is determined by the repair to be made. When soldering on circuit boards, use a 15- to 25-watt pencil-type soldering iron with a 1/8-inch wide, wedge-shaped tip. Keep the tip properly tinned for best heat transfer to the solder joint. A higher wattage soldering iron may separate the wiring from the base material. Avoid excessive heat; apply only enough heat to remove the component or to make a good solder joint. Also, apply only enough solder to make a firm solder joint; do not apply too much solder.

CAUTION

The Acquisition, Intelligence, and Button Lights circuit boards in this instrument are multilayer type boards with a conductive path(s) laminated between the top and bottom board layers. All soldering on these boards should be done with extreme care to prevent breaking the connections to the center conductor(s); only experienced maintenance personnel should attempt repair of these boards.

For metal terminals, (e.g., coaxial connector, ground lug, etc.) a higher wattage soldering iron may be required. Match the soldering iron to the work being done. For example, if the component is connected to the chassis or other large heat-radiating surface, it will require a 40-watt or larger soldering iron.

The following technique should be used to replace a component on a circuit board:

1. Grip the component lead with long-nose pliers. Touch the soldering iron to the lead at the solder connection. Do not lay the iron directly on the board, as it may damage the board.

2. When the solder begins to melt, gently pull the lead out. If unable to pull the lead out of the circuit board without using force, try removing the other end of the component as it may be more easily removed.

NOTE

The reason that some component leads seem troublesome to remove is due to a bend placed in each lead during the manufacturing process. The purpose of the bent leads is to hold the component in place during a flow-soldering manufacturing process that solders all components at one time.

If a component lead is extremely difficult to remove, it may be helpful to straighten the leads on the back side of the board with a small screwdriver or pliers while heating the soldered connection.

Unsolder the component from the circuit board using heat on the component lead so that the solder will stay behind on the board. If you desire to remove solder from a circuit board hole for easier installation of a new component, use a solder-removing wick.

3. Bend the leads of the new component to fit the holes in the board. If the component is replaced while the board is mounted in the instrument, cut the leads so they will just protrude through the board. Insert the leads into the holes in the board so the component is firmly seated against the board (or as positioned originally). If it does not seat properly, heat the solder and gently press the component into place.

4. Touch the iron to the connection and apply a small amount of solder to make a firm solder joint. To protect heat-sensitive components, hold the lead between the component body and the solder joint with a pair of long-nose pliers or other heat sink.

5. Clip the excess lead that protrudes through the board (if not clipped in step 3).

6. Clean the area around the solder connection with a flux-removing solvent. Be careful not to remove information printed on the board.

COMPONENT REMOVAL AND REPLACEMENT

WARNING

To avoid electric shock, disconnect the instrument from the power source before replacing components.

The exploded-view drawing associated with the Replaceable Mechanical Parts list may be helpful in the removal or disassembly of individual components or subassemblies. Component locations are shown in the Diagrams and Circuit Board Illustrations section.

Circuit Boards

If a circuit board is damaged beyond repair, replace the entire board assembly. Part numbers are given in the Replaceable Electrical Parts list for completely wired boards. Refer to Figure 4-4 for circuit board locations.

A2—BUTTON LIGHTS CIRCUIT BOARD. To remove the circuit board:

1. Position instrument upside down with front panel facing you. Carefully pry front panel away from sub-panel using a small screwdriver in slot provided on sub-panel bottom. Carefully remove front panel.

2. Note colors of the three multi-pin connectors and the P number to which each connects on the two front sub-panel mounted circuit board assemblies.

3. Remove 4 screws (A, B, C, and D on Fig. 4-5) from front sub-panel assembly.

4. Remove 4 screws (A, B, C, and D on Fig. 4-6) from Button Lights circuit board. Carefully lift board away from sub-panel assembly.

5. To replace Button Lights circuit board, reverse order of removal, and snap panel back into position.

A1—FORMATTER KEYBOARD CIRCUIT BOARD. To remove the circuit board:

1. Remove A2—Button Lights circuit board as previously described.

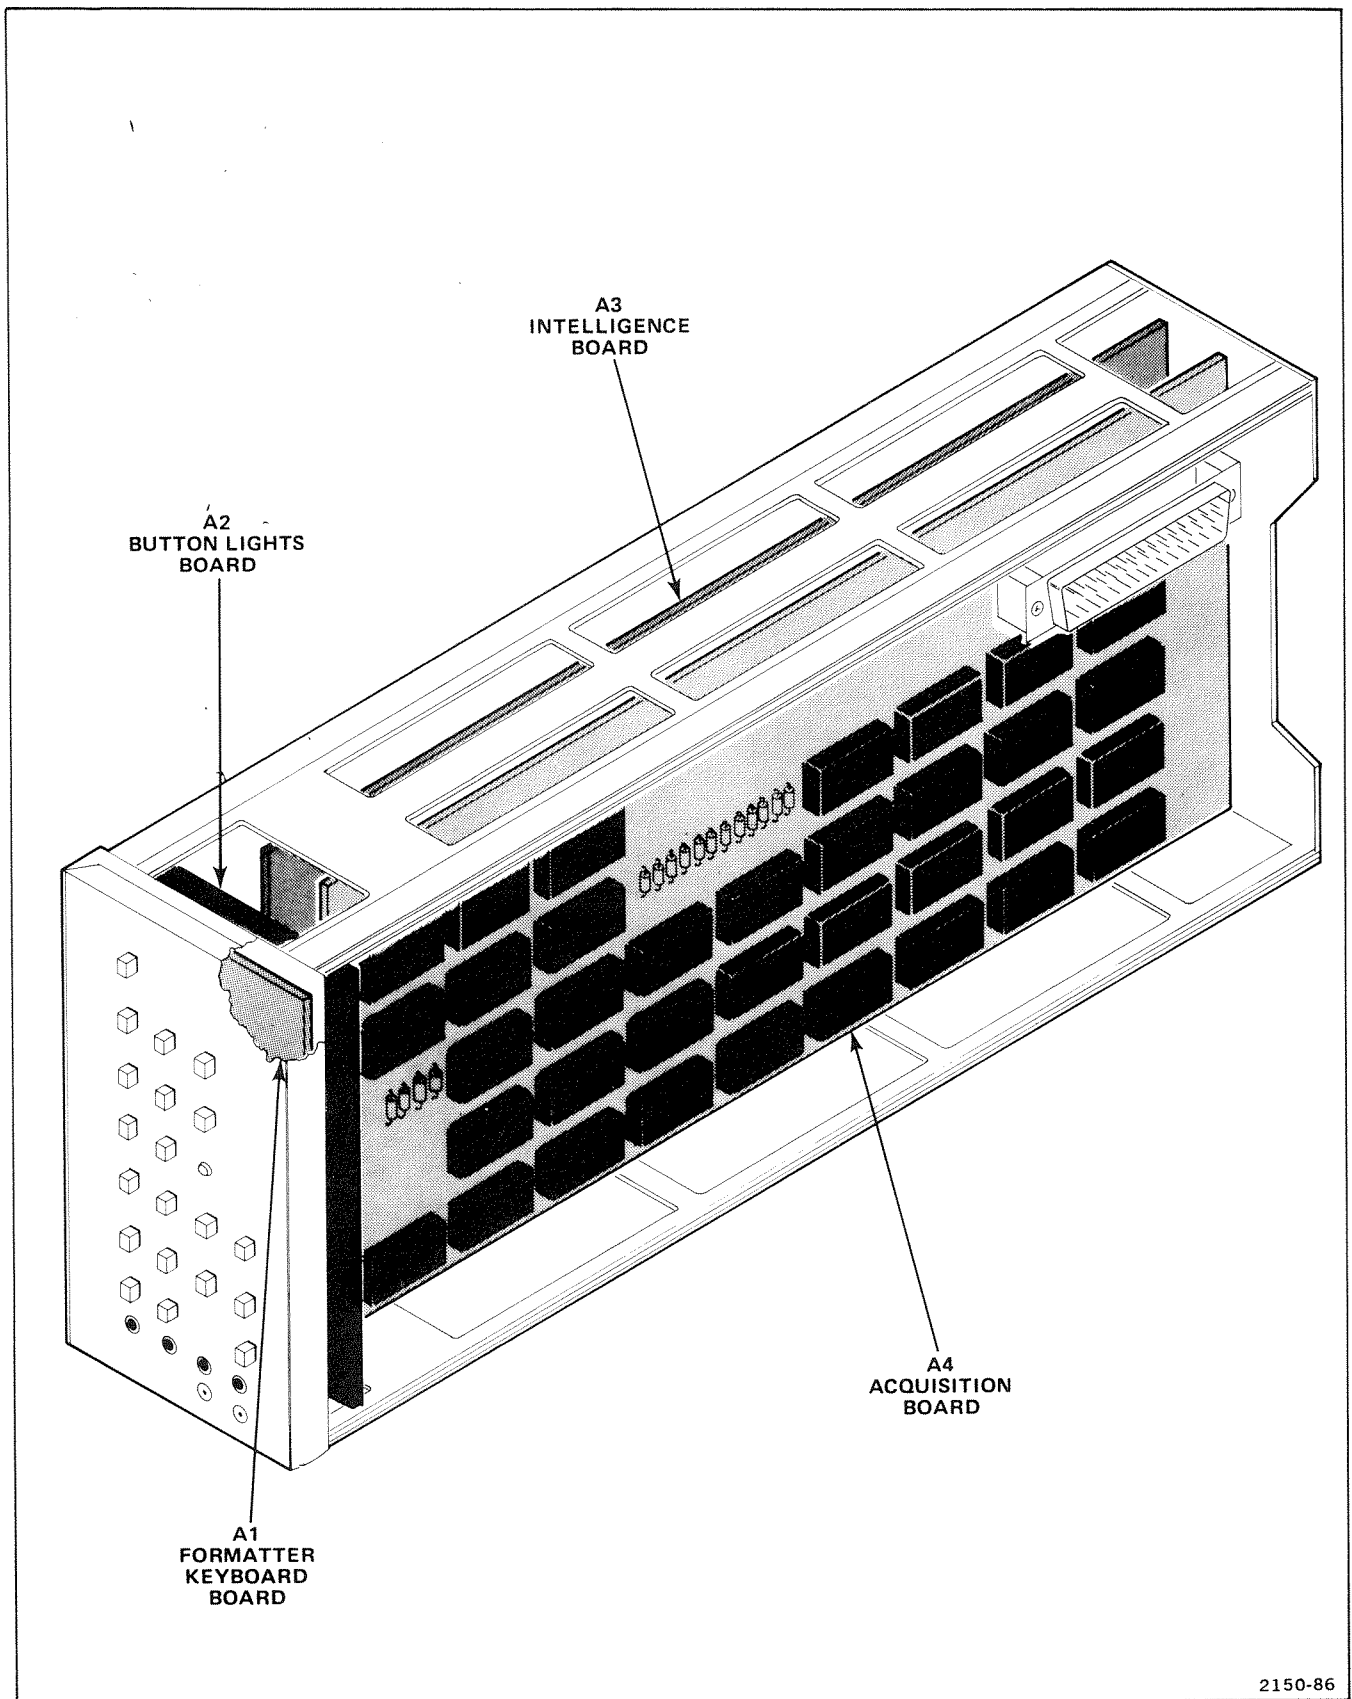


Figure 4-4. Circuit board locations.

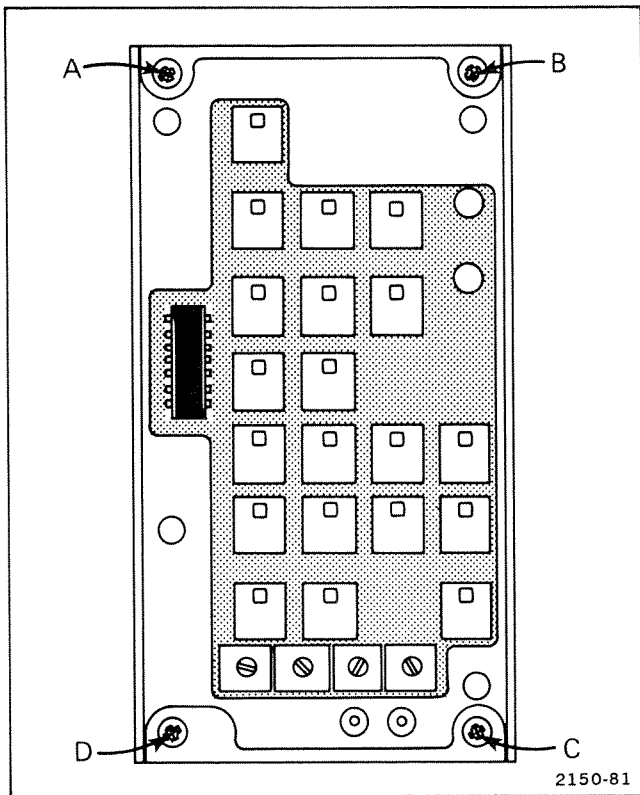


Figure 4-5. Locations of securing screws on the front sub-panel.

2. Disconnect 2 wires (W1 and W2 on Fig. 4-7). Remove 4 hexagonal spacers (A, B, C, and D on Fig. 4-7), and lift board away from front sub-panel.

3. To replace A1—Formatter Keyboard circuit board, reverse order of removal.

A3—INTELLIGENCE CIRCUIT BOARD. To remove the circuit board:

1. Remove 6 screws (A, B, C, D, E, and F on Fig. 4-8).
2. Carefully disengage interconnecting board pins (one row of interconnecting pins at front panel end of board, and one row near rear panel). Lift board clear of instrument between top and bottom frame rails.
3. To replace A3—Intelligence circuit board, reverse order of removal. The use of a small screwdriver may aid in aligning the circuit board connecting pins with their sockets.

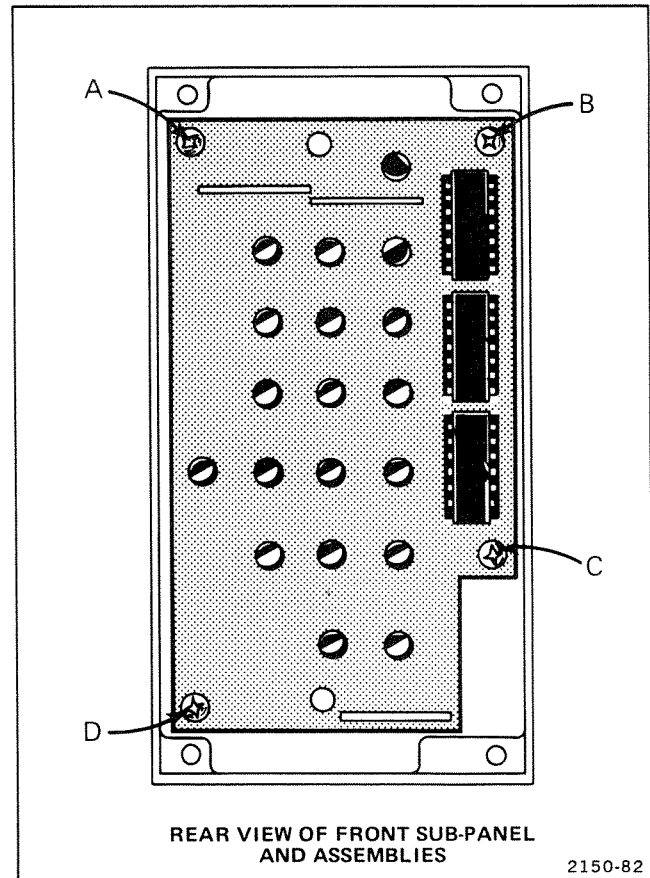


Figure 4-6. Locations of securing screws on A2 Button Lights circuit board.

A4—ACQUISITION CIRCUIT BOARD. To remove the circuit board:

1. Remove 3 screws (A, B, and C on Fig. 4-9).
2. Note color of all multi-pin connectors and the P number to which each connects.
3. Disconnect all cables that terminate on A4—Acquisition circuit board.
4. Remove 6 screws (D, E, F, G, H, and I on A4—Acquisition circuit board).
5. Carefully disengage interconnecting board pins (one row of interconnecting pins at front panel end of board, and one row near rear panel). Lift board clear of instrument between top and bottom frame rails.

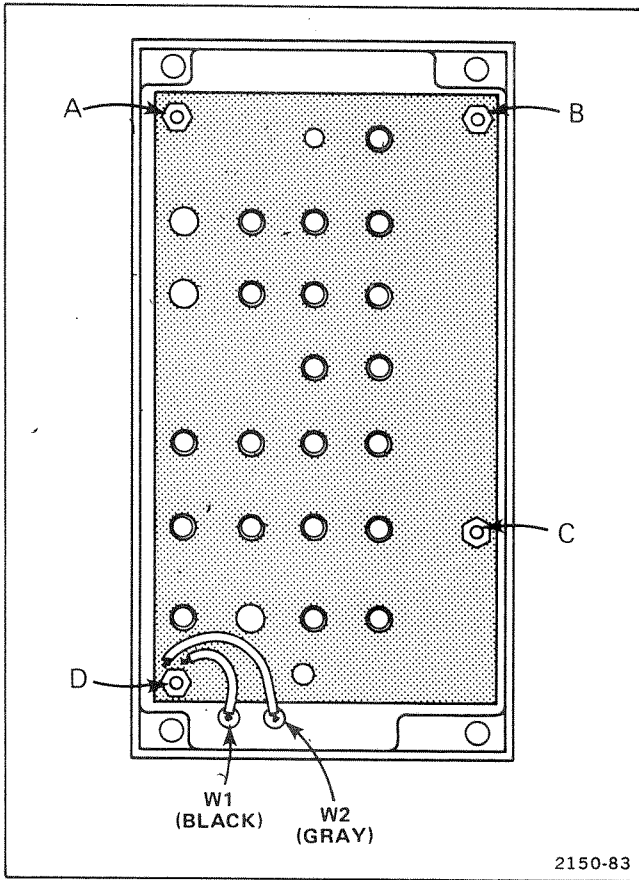


Figure 4-7. Locations of hex securing spacers and wiring to be disconnected on A1 Formatter Keyboard circuit board.

6. To replace A4—Acquisition circuit board, reverse order of removal. The use of a small screwdriver may aid in aligning the circuit board connecting pins with their sockets.

Pushbutton Switches

All the pushbutton switches used in this instrument are mounted on the A1—Formatter Keyboard circuit board. First, remove the A1—Formatter Keyboard circuit board following the procedure given under Circuit Boards in this section. To remove any switch from the board, simply push from the rear of the switch until the two plastic retainers disengage from the board. To replace the switch, align the two plastic retainers with the mating holes in the circuit board and snap into position.

Semiconductors

Semiconductors should not be replaced unless actually defective. If removed from their sockets during routine maintenance, return them to their original sockets. Unnecessary replacement of semiconductors may affect the adjustment of this instrument. When semiconductors are replaced, check the operation of the part of the instrument which may be affected.

WARNING

To avoid electric shock, power must be turned off before removing or replacing semiconductors.

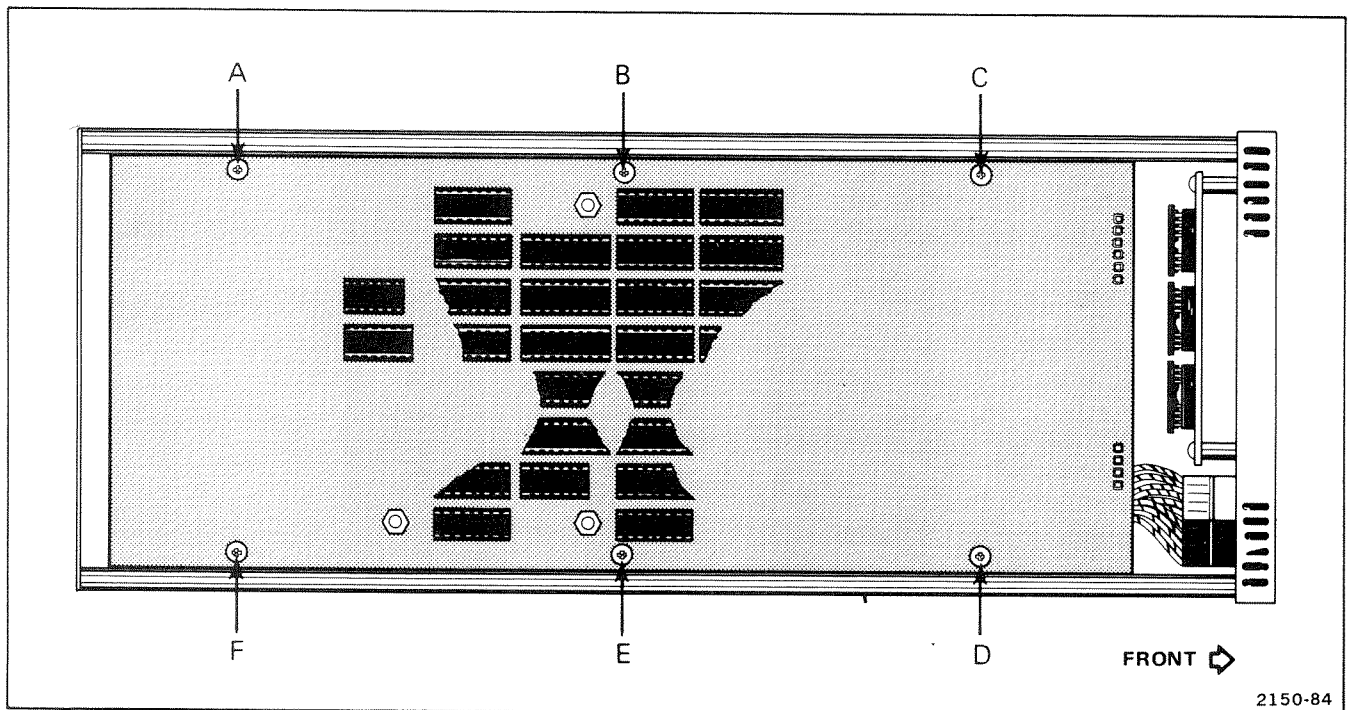


Figure 4-8. Locations of securing screws on A3 Intelligence circuit board.

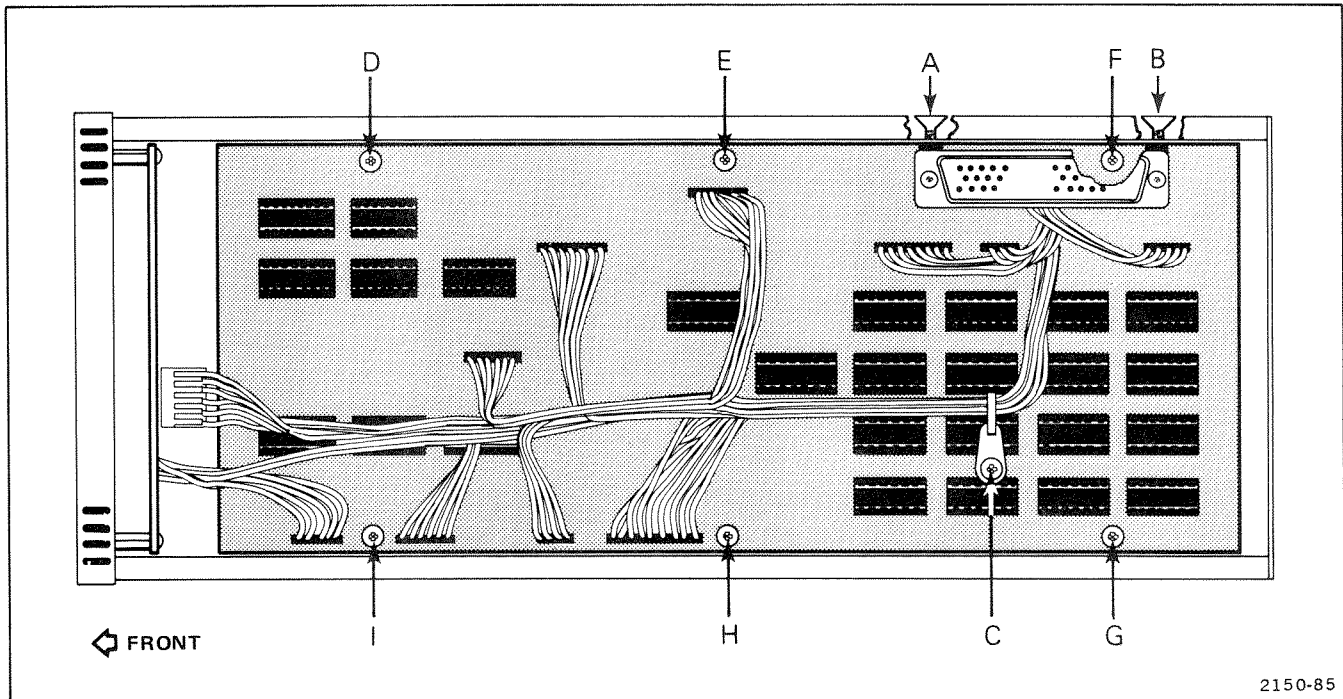


Figure 4-9. Locations of securing screws and hardware mounting screws on A4 Acquisition circuit board.

Replacement devices should be of the original type or a direct replacement. The lead configurations of the semiconductor devices used in this instrument are shown in the Diagrams and Circuit Board Illustrations section. When replacing, check the manufacturer's basing diagram for correct basing.

An extracting tool should be used to remove the 14-, 16-, 20-, and 40-pin integrated circuits to prevent damage to the pins. This tool is available from Tektronix, Inc. Order Tektronix Part 003-0619-00. If an extracting tool is not available when removing one of these integrated circuits, pull slowly and evenly on both ends of the device. Try to avoid having one end of the integrated circuit disengage from the socket before the other, as the pins may be damaged.

Interconnecting Pins

All interconnections in this instrument are made utilizing pins soldered into the board. Two types of mating connectors are used for these interconnecting pins. If the mating connector is mounted on a plug-on circuit board, a special socket is soldered into the board. If the mating connector is on the end of a lead, an end-lead pin connector is used which mates with the interconnecting pin. The following information provides the removal and replacement procedure for the various types of interconnecting methods:

CIRCUIT-BOARD PINS. A circuit-board pin replacement kit (including necessary tools, instructions, and replacement pins with attached ferrules) is available from Tektronix, Inc. Order Tektronix Part 040-0542-00. Replacing circuit-board pins on multi-layer boards is not recommended; refer such repairs to your local Tektronix Field Office or representative.

To replace a damaged pin, first disconnect any pin connectors. Then unsolder (see Soldering Techniques) the damaged pin and pull it from the board with a pair of pliers, leaving the ferrule (see Fig. 4-10) in the circuit board if possible. If the ferrule remains in the circuit board, remove the spare ferrule from the replacement pin and press the new pin into the hole in the circuit board. If the ferrule is removed with the damaged pin, clean out the hole using a solder-removing wick and a scribe. Then press the replacement pin, with attached spare ferrule, into the circuit board. Position the replacement pin in the same manner as the original pin had been. Solder the pin to the circuit board on each side of the board. If the original pin was bent at an angle to mate with a connector, carefully bend the new pin to the same angle. Replace the pin connector.

CIRCUIT-BOARD PIN SOCKETS. The pin sockets on the circuit boards are soldered to the back of the board. To remove or replace one of these sockets, first unsolder the pin (use a vacuum-type desoldering tool to remove excess

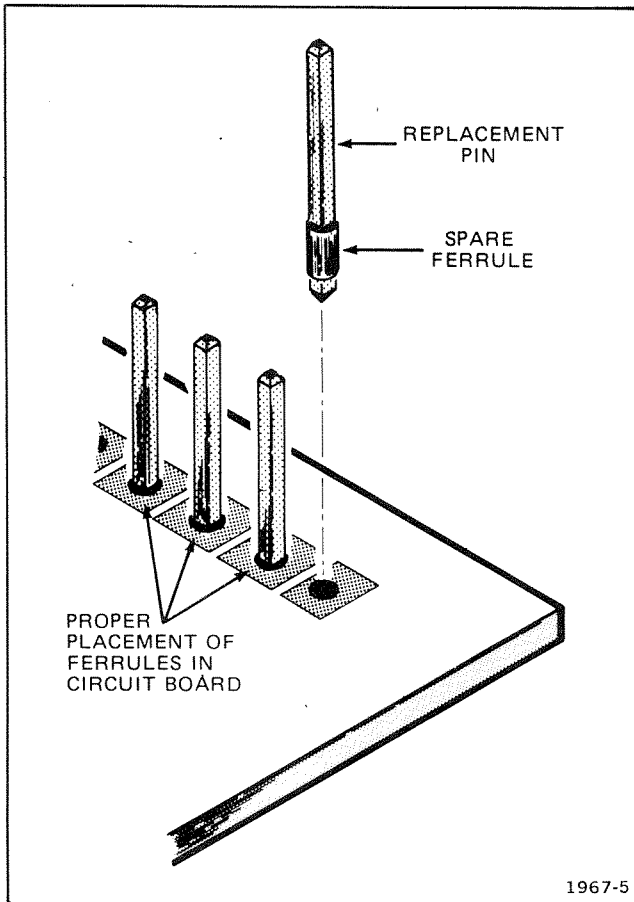


Figure 4-10. Exploded view of circuit-board pin and ferrule.

solder). Then straighten the tabs on the socket and remove the socket from the board. Place the new socket in the circuit board hole and press the tabs down against the board. Solder the tabs of the socket to the circuit board; be careful not to get solder inside the socket.

CAUTION

The spring tension of the pin sockets ensures a good connection between the circuit board and the pin. This spring tension can be destroyed by using the pin sockets as a connecting point for spring-loaded probe tips, alligator clips, etc.

END-LEAD PIN CONNECTORS. The pin connectors used to connect the wires to the interconnecting pins are clamped to the ends of the associated leads. To remove or replace damaged end-lead pin connectors, remove the old pin connector from the end of the lead and clamp the replacement connector to the lead.

Some of the pin connectors are grouped together and mounted in a plastic holder; the overall result is that these connectors are removed and installed as a multi-pin connector (see Troubleshooting Aids). If the individual end-lead pin connectors are removed from the plastic holder, note the order of the individual wires for correct replacement.

ADJUSTMENT AFTER REPAIR

After any electrical component has been replaced, the adjustment of that particular circuit should be checked, as well as other closely related circuits. See Section 5 for a complete Adjustment procedure.

PERFORMANCE CHECK AND ADJUSTMENT

This section provides information necessary to check performance requirements, functions which require removal of side panels, detailed checks of the DF1 memory, and to make internal adjustments. An additional Functional Check procedure, in the Operating Instruction section, checks the functions of the front-panel controls.

PRELIMINARY INFORMATION

Adjustment Interval

To maintain instrument accuracy, check the performance of the DF1 every 1000 hours of operation, or every 6 months if used infrequently. Before complete adjustment, thoroughly clean and inspect this instrument as outlined in section 4, Maintenance.

Tektronix Field Service

Tektronix Field Service Centers and Factory Service Centers provide instrument repair and adjustment services. Contact your Tektronix Field Office or representative for further information.

Performance Check

Performance of this instrument can be checked by performing only the Performance Check. This procedure checks the instrument against the tolerances listed in the Performance Requirement column of the DF1 Specifi-

cations, and also checks the DF1 memory. Performance Check Table 5-1 (derived from the Specifications in the General Information section) briefly describes the test method to check the performance requirement for a given characteristic. To completely check all instrument functions, as well as instrument performance, perform the Functional Check (located in the Operating Instructions section) and Performance Check procedures.

Adjustment Procedure

Completion of the Adjustment procedure ensures that the instrument is correctly adjusted. Instrument performance is checked before an adjustment is made.

Partial Procedure

A partial performance check or adjustment may be desired after replacing components or to touch up the adjustment portion of the instrument. Each Performance Check and Adjustment step is written to stand alone. Therefore to perform a partial procedure proceed to the desired numbered step (1, 2, 5, etc.) and follow the procedure.

TABLE 5-1
Performance Check Description

Characteristic	Performance Requirement	Test Method
External Read Clock Frequency Range	100 kHz to 500 kHz.	Not Tested.
Duty Cycle	50% within 5%.	Not Tested.
Display Vertical Size	Adjustable from 6.9 div, or less, to at least 8.1 div from the top of the first line of DF1 readout to the bottom of the last line of DF1 readout.	Not Tested.
Vertical Position	Adjustable to vertical center of display area in any calibrated 7000-series mainframe.	Not Tested.
Horizontal Position	Adjustable to horizontal center of display area in any calibrated 7000-series mainframe.	Not Tested.

TABLE 5-1 (CONT.)
Performance Check Description

Characteristic	Performance Requirement	Test Method
Output Signals Reset Logic Voltage Level	LO: +0.4 V, or less, at 2 mA. HI: at least +2.4 V at 2 mA.	LO tested by connecting 7D01 channel 0 probe and 2 mA source (2.4 kilohm to +5 V) to RESET OUT jack. (7D01 Threshold Voltage set to +0.4 V.) HI tested by connecting 7D01 channel 0 probe and 2 mA drain (1.2 kilohm to gnd.) to RESET OUT jack. (7D01 Threshold Voltage set to +2.4 V.)
Waveshape	Positive-going rectangular pulse.	Checked indirectly above.
Duration	100 μ s within 50 μ s when used with the 7D01 internal read clock.	Checked by using trigger-to-cursor readout on displayed pulse (1 μ s sample interval).

TEST EQUIPMENT REQUIRED

The test equipment listed in Table 5-2 is required for a complete performance check and adjustment of this instrument. The specifications for test equipment, given in Table 5-2, are the minimum required to meet the Performance Requirements. Detailed operating instructions for test equipment are omitted in this procedure. Refer to the test equipment instruction manual if more information is needed.

Special Fixtures

Special fixtures are used only where they facilitate instrument adjustment. These fixtures are available from

Tektronix, Inc. Order by part number from Tektronix Field Offices or representatives.

Test Equipment Alternatives

The test equipment listed in the Examples of Applicable Test Equipment column, Table 5-2, is required to check and adjust this instrument. The Performance Check and Adjustment procedure is based on the first item of equipment given as an example. If other equipment is substituted, control settings or setups may need to be altered. If the exact item of equipment given as an example is not available, refer to the Minimum Specifications column to determine if other equipment may be substituted. Then check the Purpose column. If you determine that your measurement requirements will not be affected, the item and corresponding step(s) can be deleted.

TABLE 5-2
Test Equipment

Description	Minimum Specifications	Purpose	Examples of Applicable Test Equipment
1. Oscilloscope mainframe	Tektronix 7000-series with 2 vertical and 1 horizontal plug-in compartments.	Provides display for 7D01 and DF1.	a. TEKTRONIX 7603 Oscilloscope. b. Refer to the TEKTRONIX catalog for a compatible oscilloscope mainframe.
2. Logic Analyzer with Data Acquisition Probes.	Tektronix 7D-series compatible with DF1.	The DF1 is operable only with a companion Logic Analyzer.	a. TEKTRONIX 7D01 Logic Analyzer with two P6451 Data Acquisition Probes.
3. TTL Signal Source	Clock and 8-bit counter. Clock frequency; approximately 1 kilohertz.	Provides standard input signals to 7D01.	a. TEKTRONIX 067-0804-00 TEST FIXTURE. b. Circuit as shown in Figure 5-2.
4. +5-Volt Power Supply	Current; at least 100 mA.	Provides power to TTL Signal Source and provides 2 mA source for Reset Out check.	a. TEKTRONIX PS501 Power Supply with TM500-series Power Module.
5. Voltmeter	Range; +0.4 V to +2.4 V.	Set 7D01 Variable Threshold Voltage during Reset Out check.	a. Triplet 630-NA VOM. b. Simpson 262.

INDEX TO PERFORMANCE CHECK AND ADJUSTMENT

	PAGE
PRELIMINARY PROCEDURE	5-3
PERFORMANCE CHECK PROCEDURE	
1. Check Trigger Points	5-4
2. Check Old Data	5-5
3. Check Data Acquisition	5-6
4. Check Mainframe Readout	5-6
5. Check Reset Out Pulse	5-7
ADJUSTMENT PROCEDURE	
1. Adjust Horizontal Gain	5-8

PRELIMINARY PROCEDURE


1. Before connecting the DF1 Display Formatter to the 7D01 Logic Analyzer, set the 7D01 for "first trigger" operation (see Fig. 5-1), and check that the DF1 is set for Formatter Readout (FOR R).

2. Attach the DF1 to the 7D01 and install the three-wide plug-in assembly into the oscilloscope mainframe (refer to Installation, in the General Information section, for assembly instructions).

3. Connect the Interface Test Fixture to the 7D01 as shown in Figure 5-2.

4. Set the 7D01 Logic Analyzer controls as follows:

- Sample Interval Ext
- Record Display Time ∞
- Data Position Post Trig
- Data Channels 0-15
- Trigger Source W.R.
- Word Recognizer
 - Ch 0 through Ch 15 Lo
 - External Qualifier X
 - Probe Qualifier X
 - W.R. Mode Sync.
- Threshold Voltage TTL (+1.4 V)
- Ext Clock Polarity \perp

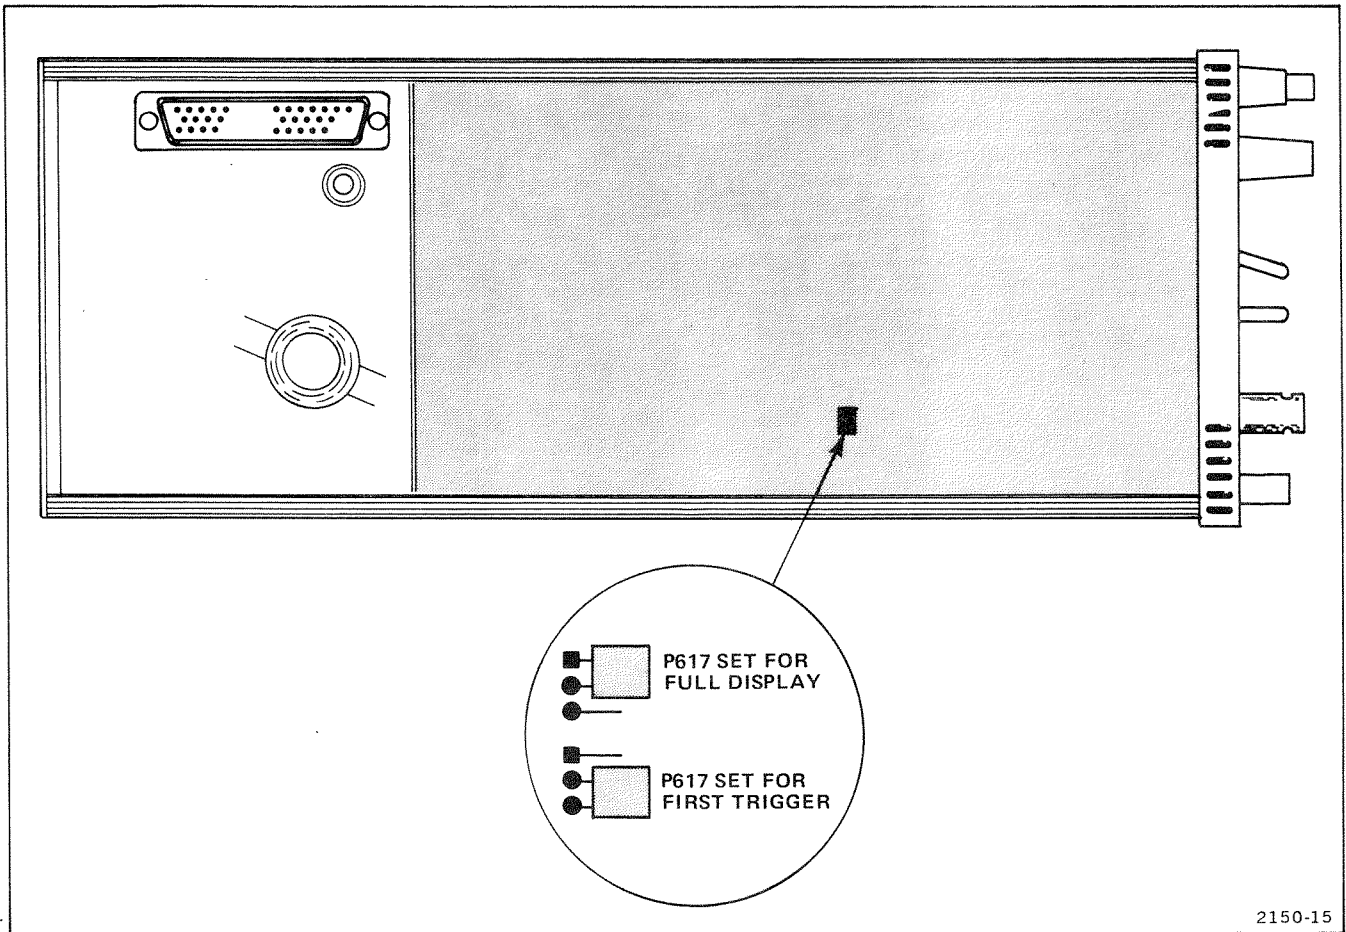

2150-15

Figure 5-1. Location of 7D01 Full Display/First Trigger jumper.

5. Perform the Power-On function (turn mainframe power off, wait approximately 10 seconds, and turn power on).

e. Set the 7D01 Cursor position controls to superimpose the cursor and trigger intensified spots on the display.

PERFORMANCE CHECK PROCEDURE

1. Check Trigger Points

a. Perform the Preliminary Procedure.

b. Adjust mainframe intensity and 7D01 Vert and Horiz controls for a well-defined Timing Diagram display.

c. Check that the trigger-to-cursor readout (top of display) is +0 and the cursor word readout (bottom of display) is 0000 0000 0000 0000 when the trigger and cursor intensified spots are superimposed.

d. Change the 7D01 Data Channels switch to 0-7 position and press the Record Manual Reset push button.

f. Check that the trigger-to-cursor readout is +0 and the cursor word readout is 0000 0000.

g. Change the 7D01 Data Channels switch to 0-3 position and press the Record Manual Reset push button.

h. Set the 7D01 Cursor position controls to superimpose the cursor and trigger intensified spots on the display.

i. Check that the trigger-to-cursor readout is +0 and that the cursor word readout is 0000.

j. Change the 7D01 Data Channels switch to 0-15 position and the Data Position switch to Center position.

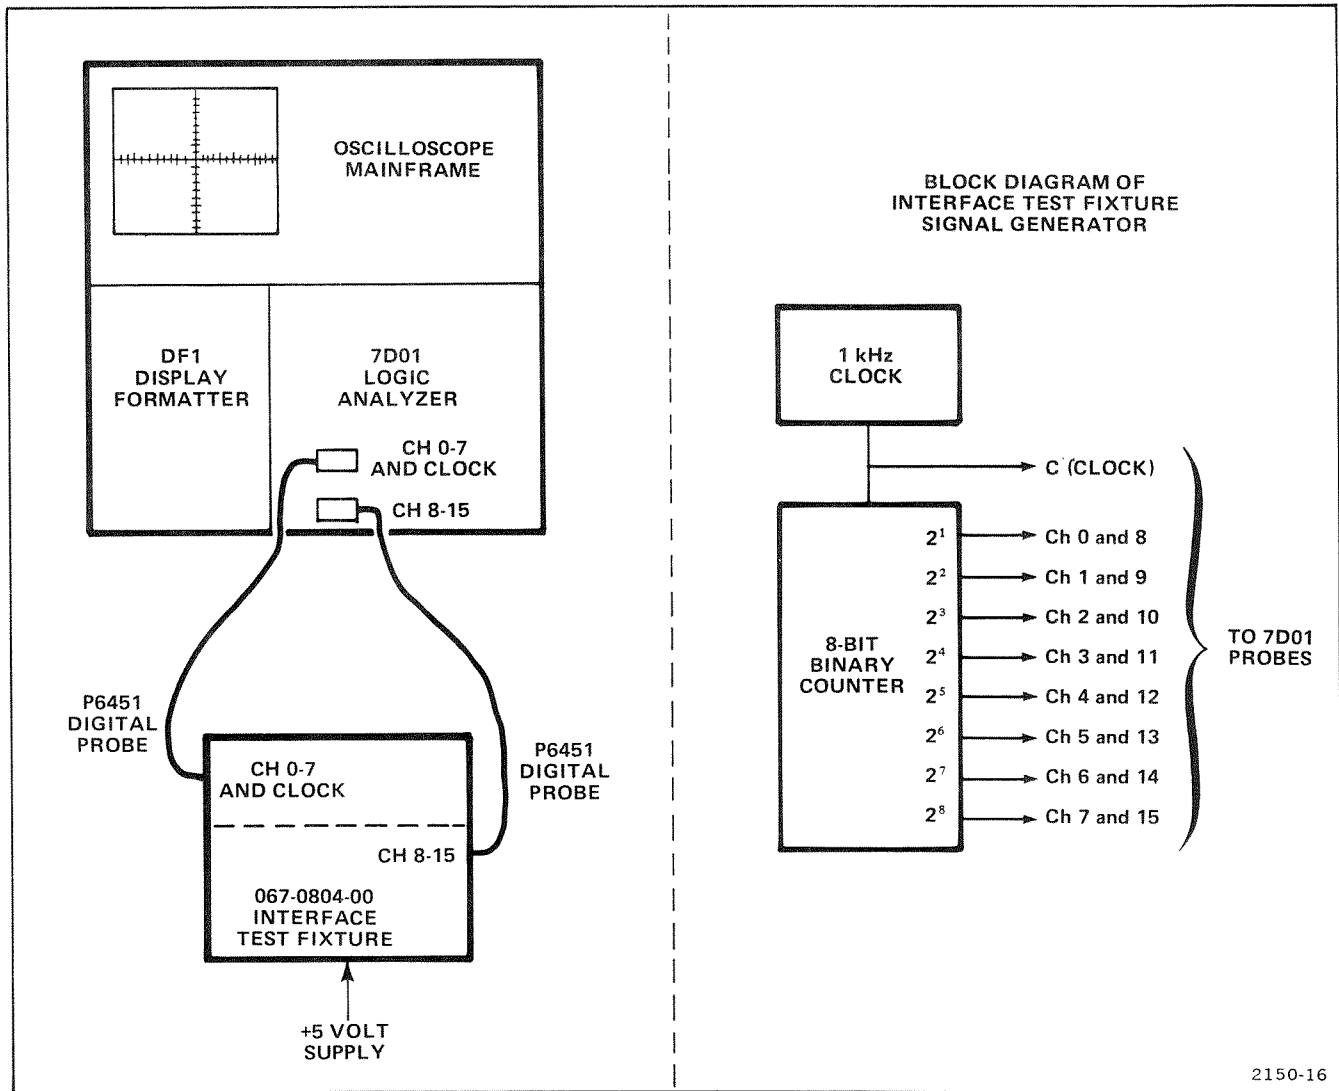


Figure 5-2. Test setup for Performance Check and Adjustment Procedure.

k. Press the Record Manual Reset push button and repeat parts c through i.

l. Change the 7D01 Data Channels switch to 0-15 position and the Data Position switch to Pre Trig position.

m. Press the Record Manual Reset push button and repeat parts c through i.

2. Check Old Data.

a. Perform Preliminary Procedure.

b. Adjust mainframe intensity and 7D01 Vert and Horiz controls for a well-defined Timing Diagram display.

c. Change 7D01 Trigger Source switch to Ch 0 position and press the Record Manual Reset push button.

d. Rotate the 7D01 Cursor Fine Pos control counter-clockwise until the cursor intensified spots disappear.

e. Check that the cursor readout (bottom of display) disappears at the same time as the cursor intensified spots.

Performance Check and Adjustment—DF1

f. Repeat parts c through e for all positions of the 7D01 Data Position and Data Channels switches.

3. Check Data Acquisition

- a. Perform the Preliminary Procedure.
- b. Press the STATE TABLE HEX push button.
- c. Adjust mainframe intensity for a well-defined display.
- d. Check that the top 16 rows of columns 1 and 3 display 0 through F (see Fig. 5-3).

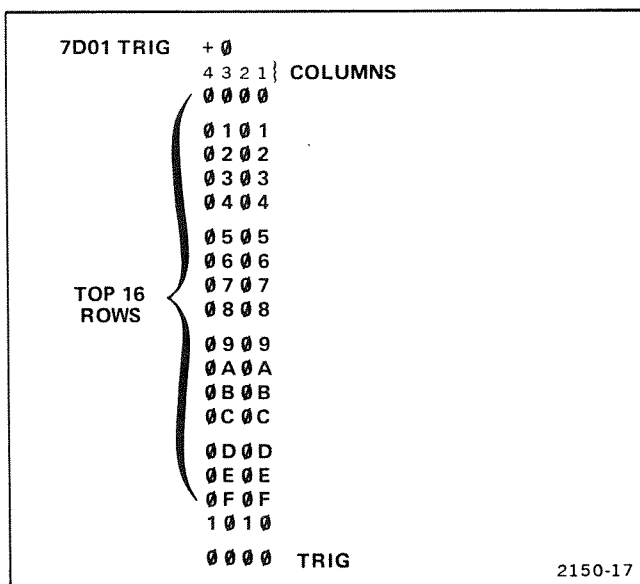


Figure 5-3. Hexadecimal State Table display.

- e. Rotate the 7D01 Cursor Coarse position switch one position clockwise at a time. Check that the data displayed in columns 1 and 3 remain the same, and that the top 16 rows of columns 2 and 4 change from all 0's (7D01 TRIG +0), to all 1's (7D01 TRIG +16), etc., through all F's (7D01 TRIG -16). Ignore any X's or *'s in the displays.
- f. Change the 7D01 Data Channels switch to 0-7 position and press the Record Manual Reset push button.
- g. Rotate the 7D01 Cursor position controls to set the trigger-to-cursor readout to +0.

h. Check that the top 16 rows of column 1 display 0 through F.

i. Rotate the 7D01 Cursor Coarse position switch one position clockwise at a time. Check that the data displayed in column 1 remain the same, and that the top 16 rows of column 2 change from all 0's through all F's twice while the trigger-to-cursor readout advances from +0 through -16. Ignore any X's or *'s in the displays.

j. Change the 7D01 Data Channels switch to 0-3 position and press the Record Manual Reset push button.

k. Rotate the 7D01 Cursor position controls to set the trigger-to-cursor readout to +0.

l. Check that the top 16 rows display 0 through F.

m. Rotate the 7D01 Cursor Coarse position switch clockwise and check that the display remains the same, while the trigger-to-cursor readout advances from +0 through -16. Ignore any X's or *'s in the display.

4. Check Mainframe Readout

- a. Perform Preliminary Procedure.
- b. Adjust mainframe intensity for a well-defined Timing Diagram display.
- c. Note the normal (formatter) readout at the top and bottom of the display.
- d. Turn off power to the mainframe and remove the 7D01-DF1 (do not disconnect the probes from the 7D01). Disconnect the DF1 from the 7D01 (refer to Installation, in the General Information section, for instructions).
- e. Set the DF1 Readout Source jumper to the MFR (mainframe readout) position.
- f. Connect the DF1 to the 7D01 and install into the mainframe.
- g. Adjust the mainframe readout intensity control and check that crt readout can be obtained.

- h. Press the MAP FAST push button and check that normal (formatter) readout is present.
- i. Press the STATE TABLE HEX push button and check that normal readout is present.
- j. Turn off power to the mainframe and remove 7D01-DF1.
- k. Disconnect the DF1 from the 7D01 and set the DF1 Readout Source jumper to FOR R (formatter readout).
- l. Reconnect the DF1 to the 7D01.


5. Check Reset Out Pulse

- a. Set the 7D01 for First Trigger mode (internal jumper). Set 7D01 controls as follows:

- Sample Interval. 1 μ s
- Record Display Time ∞
- Data Channels. 0-3
- Data Position Post Trig
- Trigger Source Ch 0
- Threshold Voltage Var (± 12 V)

Leave all probe tips open.

- b. Turn on power to mainframe.
- c. Press 7D01 Manual Trigger push button and adjust mainframe intensity and 7D01 Vert and Horiz controls for a well-defined Timing Diagram display (four traces).
- d. Connect a voltmeter between the 7D01 Threshold Voltage Monitor jack and ground and set to +2.4 volts.
- e. Connect a 1.2-kilohm resistor between the DF1 RESET OUT jack and ground (Figure 5-4A).
- f. Connect the Channel 0 probe tip to the RESET OUT jack.
- g. Press the RESET IF 7D01=REF push button and check that the 7D01 resets once and displays a HI pulse on channel 0 of the Timing Diagram.

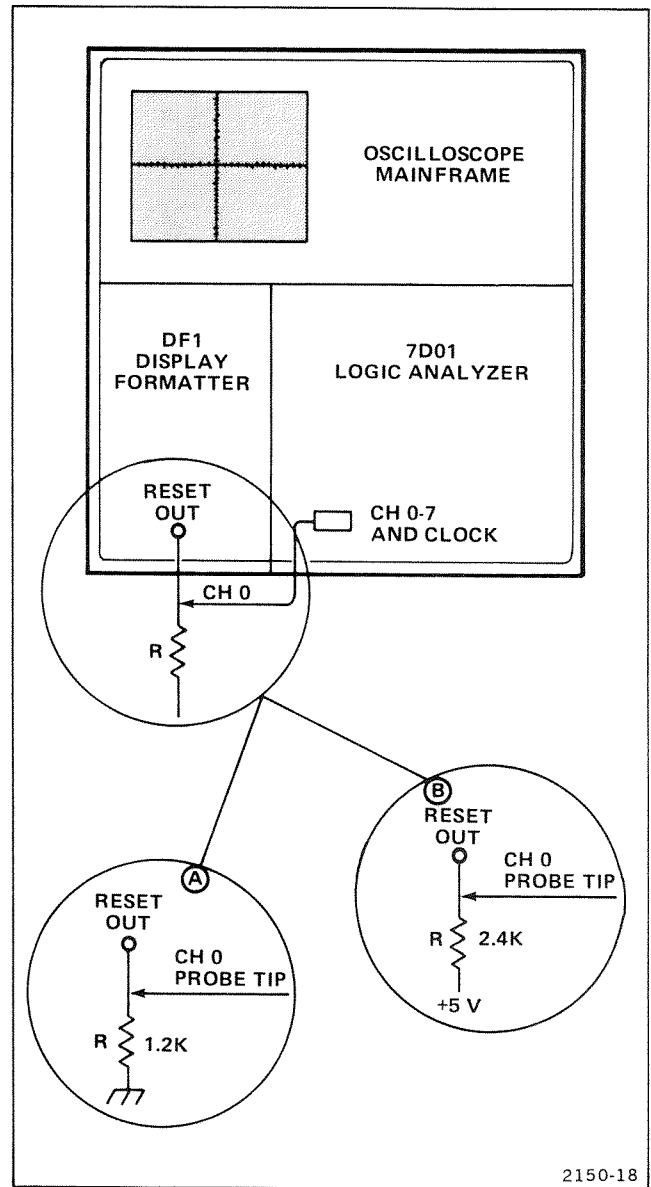

2150-18

Figure 5-4. Reset Out check test setup.

- h. Rotate the 7D01 Cursor position controls to set the cursor intensified dot to the falling edge of the displayed pulse.
- i. Check that the trigger-to-cursor readout is at least +50 and less than or equal to +150.
- j. Set the 7D01 Threshold Voltage Monitor for +0.4 volts.
- k. Disconnect the 1.2-kilohm resistor and Channel 0 probe from the RESET OUT jack.

Performance Check and Adjustment—DF1

- l. Press the 7D01 Record Manual Reset and Manual Trigger push buttons (in that order).
- m. Connect a 2.4-kilohm resistor from a +5-volt supply to the RESET OUT jack (figure 5-4B).
- n. Connect the Channel 0 probe to the RESET OUT jack.
- o. Press the RESET IF 7D01=REF push button and check that the 7D01 resets once and displays a HI pulse on channel 0 of the Timing Diagram display.
- p. Disconnect the 2.4-kilohm resistor and Channel 0 probe from the RESET OUT jack.
- q. Turn off power to the mainframe and remove the 7D01-DF1.
- r. Disconnect the DF1 from the 7D01 and set the 7D01 to the Full Display mode (internal jumper).
- b. Press MAP FAST push button and adjust mainframe intensity control for well-defined Map display (diagonal line).
- c. Adjust the front-panel HORIZ POSN screwdriver adjustment to position the left end of the Map display to the left edge of the crt graticule.
- d. Note the position of the right end of the Map display relative to the edge of the crt graticule. The right end of the display should be within 0.2 division from the right edge of the graticule.
- e. If adjustment of the horizontal gain is required; turn off the power to the mainframe, partially remove the 7D01-DF1 from the mainframe, and adjust the Horiz Gain screwdriver adjustment (accessible through the top rail of the DF1). (Clockwise rotation of the control reduces the horizontal gain.)
- f. Check the resultant adjustment by re-inserting the 7D01-DF1 into the mainframe, applying power, and pressing the MAP FAST push button.
- g. Repeat parts e and f as required.

ADJUSTMENT PROCEDURE

1. Adjust Horizontal Gain

- a. Perform the Preliminary Procedure. (Do NOT set 7D01 to First Trigger mode.)

REPLACEABLE ELECTRICAL PARTS

PARTS ORDERING INFORMATION

Replacement parts are available from or through your local Tektronix, Inc. Field Office or representative.

Changes to Tektronix instruments are sometimes made to accommodate improved components as they become available, and to give you the benefit of the latest circuit improvements developed in our engineering department. It is therefore important, when ordering parts, to include the following information in your order: Part number, instrument type or number, serial number, and modification number if applicable.

If a part you have ordered has been replaced with a new or improved part, your local Tektronix, Inc. Field Office or representative will contact you concerning any change in part number.

Change information, if any, is located at the rear of this manual.

SPECIAL NOTES AND SYMBOLS

X000	Part first added at this serial number
00X	Part removed after this serial number

ITEM NAME

In the Parts List, an Item Name is separated from the description by a colon (:). Because of space limitations, an Item Name may sometimes appear as incomplete. For further Item Name identification, the U.S. Federal Cataloging Handbook H6-1 can be utilized where possible.

ABBREVIATIONS

ACTR	ACTUATOR	PLSTC	PLASTIC
ASSY	ASSEMBLY	QTZ	QUARTZ
CAP	CAPACITOR	RECP	RECEPTACLE
CER	CERAMIC	RES	RESISTOR
CKT	CIRCUIT	RF	RADIO FREQUENCY
COMP	COMPOSITION	SEL	SELECTED
CONN	CONNECTOR	SEMICOND	SEMICONDUCTOR
ELCTLT	ELECTROLYTIC	SENS	SENSITIVE
ELEC	ELECTRICAL	VAR	VARIABLE
INCAND	INCANDESCENT	WW	WIREWOUND
LED	LIGHT EMITTING DIODE	XFMR	TRANSFORMER
NONWIR	NON WIREWOUND	XTAL	CRYSTAL

Replaceable Electrical Parts—DF1

CROSS INDEX—MFR. CODE NUMBER TO MANUFACTURER

Mfr. Code	Manufacturer	Address	City, State, Zip
0000W	UNITED CHEMICON, INC.	731 JAMES STREET	SYRACUSE, NY 13203
01121	ALLEN-BRADLEY COMPANY	1201 2ND STREET SOUTH	MILWAUKEE, WI 53204
01295	TEXAS INSTRUMENTS, INC., SEMICONDUCTOR GROUP	P O BOX 5012, 13500 N CENTRAL EXPRESSWAY	DALLAS, TX 75222
04713	MOTOROLA, INC., SEMICONDUCTOR PROD. DIV.	5005 E MCDOWELL RD, PO BOX 20923	PHOENIX, AZ 85036
07263	FAIRCHILD SEMICONDUCTOR, A DIV. OF FAIRCHILD CAMERA AND INSTRUMENT CORP.	464 ELLIS STREET	MOUNTAIN VIEW, CA 94042
07910	TELEDYNE SEMICONDUCTOR	12515 CHADRON AVE.	HAWTHORNE, CA 90250
14752	ELECTRO CUBE INC.	1710 S. DEL MAR AVE.	SAN GABRIEL, CA 91776
18324	SIGNETICS CORP.	811 E. ARQUES	SUNNYVALE, CA 94086
27014	NATIONAL SEMICONDUCTOR CORP.	2900 SEMICONDUCTOR DR.	SANTA CLARA, CA 95051
32997	BOURNS, INC., TRIMPOT PRODUCTS DIV.	1200 COLUMBIA AVE.	RIVERSIDE, CA 92507
34649	INTEL CORP.	3065 BOWERS AVE.	SANTA CLARA, CA 95051
50579	LITRONIX INC.	19000 HOMESTEAD RD.	CUPERTINO, CA 95014
53184	XCITON CORPORATION	5 HEMLOCK STREET	LATHAM, NY 12110
56289	SPRAGUE ELECTRIC CO.		NORTH ADAMS, MA 01247
72982	ERIE TECHNOLOGICAL PRODUCTS, INC.	644 W. 12TH ST.	ERIE, PA 16512
73138	BECKMAN INSTRUMENTS, INC., HELIPOT DIV.	2500 HARBOR BLVD.	FULLERTON, CA 92634
75042	TRW ELECTRONIC COMPONENTS, IRC FIXED RESISTORS, PHILADELPHIA DIVISION	401 N. BROAD ST.	PHILADELPHIA, PA 19108
80009	TEKTRONIX, INC.	P. O. BOX 500	BEAVERTON, OR 97077
91637	DALE ELECTRONICS, INC.	P. O. BOX 609	COLUMBUS, NE 68601

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
A1	670-4663-00			CKT BOARD ASSY:KEYBOARD	80009	670-4663-00
A2	670-4664-00			CKT BOARD ASSY:BUTTON LIGHTS	80009	670-4664-00
A3	670-4662-00			CKT BOARD ASSY:INTELLIGENCE	80009	670-4662-00
A4	670-4661-00			CKT BOARD ASSY:ACQUISITION	80009	670-4661-00
C72	290-0745-00			CAP.,FXD,ELCTLT:22UF,+50-10%,25V	56289	502D225
C73	290-0746-00			CAP.,FXD,ELCTLT:47UF,+50-10%,16V	0000W	16VBSL47
C74	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C75	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C76	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C77	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C78	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C79	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C81	290-0746-00			CAP.,FXD,ELCTLT:47UF,+50-10%,16V	0000W	16VBSL47
C82	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C83	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C84	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C85	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C86	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C87	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C93	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C95	290-0745-00			CAP.,FXD,ELCTLT:22UF,+50-10%,25V	56289	502D225
C96	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C97	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C98	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C99	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C187	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C206	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C233	281-0772-00			CAP.,FXD,CER DI:0.0047UF,10%,100V	72982	8005H9AADW5R472K
C243	281-0772-00			CAP.,FXD,CER DI:0.0047UF,10%,100V	72982	8005H9AADW5R472K
C254	290-0745-00			CAP.,FXD,ELCTLT:22UF,+50-10%,25V	56289	502D225
C257	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C310	281-0786-00			CAP.,FXD,CER DI:150PF,10%,100V	72982	390-049X5P151K
C311	281-0786-00			CAP.,FXD,CER DI:150PF,10%,100V	72982	390-049X5P151K
C467	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C468	281-0762-00			CAP.,FXD,CER DI:27PF,20%,100V	72982	390-049X5P0270M
C470	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C472	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C481	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C492	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C493	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C494	290-0782-00			CAP.,FXD,ELCTLT:4.7UF,+75-10%,35V	56289	503D475G035AS
C567	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C568	281-0762-00			CAP.,FXD,CER DI:27PF,20%,100V	72982	390-049X5P0270M
C570	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C572	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C581	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C583	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C604	281-0759-00			CAP.,FXD,CER DI:22PF,10%,100V	72982	390-049X5P0220K
C605	281-0759-00			CAP.,FXD,CER DI:22PF,10%,100V	72982	390-049X5P0220K
C624	281-0788-00			CAP.,FXD,CER DI:470PF,10%,100V	72982	8005H9AADW5R471K
C625	281-0788-00			CAP.,FXD,CER DI:470PF,10%,100V	72982	8005H9AADW5R471K
C641	285-1076-00			CAP.,FXD,PLASTIC:0.2UF,5%,100V	14752	230B1B204J
C642	281-0773-00			CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C691	281-0785-00			CAP.,FXD,CER DI:68PF,10%,100V	72982	390-049X5P680K
C704	281-0791-00	B010100	B010219	CAP.,FXD,CER DI:270PF,10%,100V	80009	281-0791-00
C704	281-0773-00	B010220		CAP.,FXD,CER DI:0.01UF,10%,100V	72982	8005H9AADW5R103K
C705	281-0762-00	B010100	B010219X	CAP.,FXD,CER DI:27PF,20%,100V	72982	390-049X5P0270M
C706	283-0115-00	XB010220		CAP.,FXD,CER DI:47PF,5%,200V	72982	805-509C0G470J
C748	281-0786-00			CAP.,FXD,CER DI:150PF,10%,100V	72982	390049X5P0151K

Replaceable Electrical Parts—DF1

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
C749	281-0786-00			CAP.,FXD,CER DI:150PF,10%,100V	72982	390-049X5P151K
CR62	152-0107-00			SEMICON D DEVICE:SILICON,400V,400MA	80009	152-0107-00
CR151	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
CR152	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
CR254	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
CR471	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
CR564	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
CR565	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
CR571	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
CR691	152-0141-02			SEMICON D DEVICE:SILICON,30V,150MA	07910	1N4152
DS8	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS10	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS12	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS14	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS18	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS20	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS22	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS26	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS28	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS30	150-1029-00			LAMP,LED:2.0V,GREEN	53184	XC209G
DS34	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS36	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS38	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS40	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS42	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS44	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS46	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS52	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
DS54	150-1036-00			LAMP,LED:RED,3.0V,40MA	50579	RL4484
L73	108-0574-00			COIL,RF:30UH	80009	108-0574-00
L81	108-0574-00			COIL,RF:30UH	80009	108-0574-00
L704	108-0736-00	B010100	B010219X	COIL,RF:825NH	80009	108-0736-00
LR72	108-0184-00			COIL,RF:3.2UH(WOUND ON A 10 OHM RESISTOR)	80009	108-0184-00
LR95	108-0184-00			COIL,RF:3.2UH(WOUND ON A 10 OHM RESISTOR)	80009	108-0184-00
Q8	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q10	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q12	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q14	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q18	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q20	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q22	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q26	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q28	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q30	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q34	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q36	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q38	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q40	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q42	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q44	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q46	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
Q52	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q54	151-0254-00			TRANSISTOR:SILICON,NPN	80009	151-0254-00
Q141	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q151	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q184	151-0342-00			TRANSISTOR:SILICON,PNP	80009	151-0342-00
Q188	151-0342-00			TRANSISTOR:SILICON,PNP	80009	151-0342-00
Q202	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q206	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q234	151-0342-00			TRANSISTOR:SILICON,PNP	80009	151-0342-00
Q244	151-0342-00			TRANSISTOR:SILICON,PNP	80009	151-0342-00
Q254	151-0342-00			TRANSISTOR:SILICON,PNP	80009	151-0342-00
Q258	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q472	151-0460-00			TRANSISTOR:SILICON,NPN	07263	2N3947
Q482	151-0460-00			TRANSISTOR:SILICON,NPN	07263	2N3947
Q486	151-0459-00			TRANSISTOR:SILICON,PNP	04713	2N3251
Q572	151-0460-00			TRANSISTOR:SILICON,NPN	07263	2N3947
Q582	151-0459-00			TRANSISTOR:SILICON,PNP	04713	2N3251
Q586	151-0459-00			TRANSISTOR:SILICON,PNP	04713	2N3251
Q592	151-0342-00			TRANSISTOR:SILICON,PNP	80009	151-0342-00
Q594	156-0065-00			MICROCIRCUIT,LI:FIVE NPN TRANSISTOR ARRAY	80009	156-0065-00
Q752	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q754	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q756	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q760	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q762	151-0223-00			TRANSISTOR:SILICON,NPN	80009	151-0223-00
Q764	151-0220-00			TRANSISTOR:SILICON,PNP	80009	151-0220-00
Q770	151-0341-00			TRANSISTOR:SILICON,NPN	07263	S040065
Q772	151-0223-00			TRANSISTOR:SILICON,NPN	80009	151-0223-00
Q774	151-0220-00			TRANSISTOR:SILICON,PNP	80009	151-0220-00
Q782	151-0342-00			TRANSISTOR:SILICON,PNP	80009	151-0342-00
Q792	151-0435-00			TRANSISTOR:SILICON,PNP	04713	MPS-A65
Q794	156-0065-00			MICROCIRCUIT,LI:FIVE NPN TRANSISTOR ARRAY	80009	156-0065-00
Q796	151-0435-00			TRANSISTOR:SILICON,PNP	04713	MPS-A65
R8	315-0101-00			RES.,FXD,CMPSN:100 OHM,5%,0.25W	01121	CB1015
R9	307-0489-00			RES,NTWK,FXD,FI:THICK FILM,100 OHM,20%,1W	32997	4408R0011010
R19	307-0489-00			RES,NTWK,FXD,FI:THICK FILM,100 OHM,20%,1W	32997	4408R0011010
R21	315-0104-00			RES.,FXD,CMPSN:100K OHM,5%,0.25W	01121	CB1045
R29	307-0489-00			RES,NTWK,FXD,FI:THICK FILM,100 OHM,20%,1W	32997	4408R0011010
R30	315-0101-00			RES.,FXD,CMPSN:100 OHM,5%,0.25W	01121	CB1015
R39	315-0104-00			RES.,FXD,CMPSN:100K OHM,5%,0.25W	01121	CB1045
R40	315-0101-00			RES.,FXD,CMPSN:100 OHM,5%,0.25W	01121	CB1015
R62	303-0360-00			RES.,FXD,CMPSN:36 OHM,5%,1W	01121	GB3605
R65	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R66	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R67	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R68	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R141	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R142	315-0202-00			RES.,FXD,CMPSN:2K OHM,5%,0.25W	01121	CB2025
R150	315-0133-00			RES.,FXD,CMPSN:13K OHM,5%,0.25W	01121	CB1335
R151	315-0391-00			RES.,FXD,CMPSN:390 OHM,5%,0.25W	01121	CB3915
R152	315-0620-00			RES.,FXD,CMPSN:62 OHM,5%,0.25W	01121	CB6205
R156	315-0512-00			RES.,FXD,CMPSN:5.1K OHM,5%,0.25W	01121	CB5125
R184	315-0201-00			RES.,FXD,CMPSN:200 OHM,5%,0.25W	01121	CB2015

Replaceable Electrical Parts—DF1

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
R187	315-0132-00			RES.,FXD,CMPSN:1.3K OHM,5%,0.25W	01121	CB1325
R188	315-0362-00			RES.,FXD,CMPSN:3.6K OHM,5%,0.25W	01121	CB3625
R201	315-0101-00			RES.,FXD,CMPSN:100 OHM,5%,0.25W	01121	CB1015
R202	315-0681-00			RES.,FXD,CMPSN:680 OHM,5%,0.25W	01121	CB6815
R203	315-0162-00			RES.,FXD,CMPSN:1.6K OHM,5%,0.25W	01121	CB1625
R204	315-0132-00			RES.,FXD,CMPSN:1.3K OHM,5%,0.25W	01121	CB1325
R205	315-0153-00			RES.,FXD,CMPSN:15K OHM,5%,0.25W	01121	CB1535
R206	315-0681-00			RES.,FXD,CMPSN:680 OHM,5%,0.25W	01121	CB6815
R232	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R233	315-0221-00			RES.,FXD,CMPSN:220 OHM,5%,0.25W	01121	CB2215
R234	315-0100-00			RES.,FXD,CMPSN:10 OHM,5%,0.25W	01121	CB1005
R235	315-0220-00			RES.,FXD,CMPSN:22 OHM,5%,0.25W	01121	CB2205
R242	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R243	315-0221-00			RES.,FXD,CMPSN:220 OHM,5%,0.25W	01121	CB2215
R244	315-0100-00			RES.,FXD,CMPSN:10 OHM,5%,0.25W	01121	CB1005
R245	315-0220-00			RES.,FXD,CMPSN:22 OHM,5%,0.25W	01121	CB2205
R251	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R252	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R254	315-0511-00			RES.,FXD,CMPSN:510 OHM,5%,0.25W	01121	CB5115
R255	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R256	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R257	315-0472-00			RES.,FXD,CMPSN:4.7K OHM,5%,0.25W	01121	CB4725
R258	315-0222-00			RES.,FXD,CMPSN:2.2K OHM,5%,0.25W	01121	CB2225
R259	315-0472-00			RES.,FXD,CMPSN:4.7K OHM,5%,0.25W	01121	CB4725
R262	315-0242-00			RES.,FXD,CMPSN:2.4K OHM,5%,0.25W	01121	CB2425
R263	315-0472-00			RES.,FXD,CMPSN:4.7K OHM,5%,0.25W	01121	CB4725
R284	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R310	315-0752-00			RES.,FXD,CMPSN:7.5K OHM,5%,0.25W	01121	CB7525
R311	315-0752-00			RES.,FXD,CMPSN:7.5K OHM,5%,0.25W	01121	CB7525
R463	315-0182-00			RES.,FXD,CMPSN:1.8K OHM,5%,0.25W	01121	CB1825
R467	315-0200-00			RES.,FXD,CMPSN:20 OHM,5%,0.25W	01121	CB2005
R469	315-0162-00			RES.,FXD,CMPSN:1.6K OHM,5%,0.25W	01121	CB1625
R470	311-1248-00			RES.,VAR,NONWIR:500 OHM,10%,0.50W	73138	72X-23-0-501K
R471	315-0752-00			RES.,FXD,CMPSN:7.5K OHM,5%,0.25W	01121	CB7525
R472	315-0163-00			RES.,FXD,CMPSN:16K OHM,5%,0.25W	01121	CB1635
R475	311-1228-00			RES.,VAR,NONWIR:10K OHM,20%,0.50W	32997	3386F-T04-103
R480	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R481	315-0101-00			RES.,FXD,CMPSN:100 OHM,5%,0.25W	01121	CB1015
R482	315-0331-00			RES.,FXD,CMPSN:330 OHM,5%,0.25W	01121	CB3315
R483	323-0195-00			RES.,FXD,FILM:1.05K OHM,1%,0.50W	75042	CECT0-1051F
R484	321-0108-00			RES.,FXD,FILM:130 OHM,1%,0.125W	91637	MFF1816G130ROF
R485	321-0155-00			RES.,FXD,FILM:402 OHM,1%,0.125W	91637	MFF1816G402ROF
R486	315-0201-00			RES.,FXD,CMPSN:200 OHM,5%,0.25W	01121	CB2015
R491	321-0270-00			RES.,FXD,FILM:6.34K OHM,1%,0.125W	91637	MFF1816G63400F
R492	321-0222-00			RES.,FXD,FILM:2K OHM,1%,0.125W	91637	MFF1816G20000F
R494	315-0361-00			RES.,FXD,CMPSN:360 OHM,5%,0.25W	01121	CB3615
R495	315-0300-00			RES.,FXD,CMPSN:30 OHM,5%,0.25W	01121	CB3005
R502	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R503	315-0512-00			RES.,FXD,CMPSN:5.1K OHM,5%,0.25W	01121	CB5125
R505	315-0513-00			RES.,FXD,CMPSN:51K OHM,5%,0.25W	01121	CB5135
R506	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R508	315-0154-00			RES.,FXD,CMPSN:150K OHM,5%,0.25W	01121	CB1545
R562	315-0124-00			RES.,FXD,CMPSN:120K OHM,5%,0.25W	01121	CB1245

Replaceable Electrical Parts—DF1

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
R563	315-0182-00			RES.,FXD,CMPSN:1.8K OHM,5%,0.25W	01121	CB1825
R564	315-0472-00			RES.,FXD,CMPSN:4.7K OHM,5%,0.25W	01121	CB4725
R565	315-0273-00			RES.,FXD,CMPSN:27K OHM,5%,0.25W	01121	CB2735
R566	315-0223-00			RES.,FXD,CMPSN:22K OHM,5%,0.25W	01121	CB2235
R567	315-0200-00			RES.,FXD,CMPSN:20 OHM,5%,0.25W	01121	CB2005
R569	315-0162-00			RES.,FXD,CMPSN:1.6K OHM,5%,0.25W	01121	CB1625
R570	311-1225-00			RES.,VAR,NONWIR:1K OHM,20%,0.50W	32997	3386F-T04-102
R571	315-0752-00			RES.,FXD,CMPSN:7.5K OHM,5%,0.25W	01121	CB7525
R572	315-0133-00			RES.,FXD,CMPSN:13K OHM,5%,0.25W	01121	CB1335
R575	311-1128-00			RES.,VAR,NONWIR:10K OHM,20%,0.50W	32997	3386F-T04-103
R580	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R581	315-0101-00			RES.,FXD,CMPSN:100 OHM,5%,0.25W	01121	CB1015
R582	315-0331-00			RES.,FXD,CMPSN:330 OHM,5%,0.25W	01121	CB3315
R583	323-0195-00			RES.,FXD,FILM:1.05K OHM,1%,0.50W	75042	CECT0-1051F
R584	321-0108-00			RES.,FXD,FILM:130 OHM,1%,0.125W	91637	MFF1816G130R0F
R585	321-0155-00			RES.,FXD,FILM:402 OHM,1%,0.125W	91637	MFF1816G402R0F
R586	315-0201-00			RES.,FXD,CMPSN:200 OHM,5%,0.25W	01121	CB2015
R590	315-0113-00			RES.,FXD,CMPSN:11K OHM,5%,0.25W	01121	CB1135
R591	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R592	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R594	315-0361-00			RES.,FXD,CMPSN:360 OHM,5%,0.25W	01121	CB3615
R595	315-0300-00			RES.,FXD,CMPSN:30 OHM,5%,0.25W	01121	CB3005
R604	315-0622-00			RES.,FXD,CMPSN:6.2K OHM,5%,0.25W	01121	CB6225
R605	315-0432-00			RES.,FXD,CMPSN:4.3K OHM,5%,0.25W	01121	CB4325
R624	315-0472-00			RES.,FXD,CMPSN:4.7K OHM,5%,0.25W	01121	CB4725
R625	315-0153-00			RES.,FXD,CMPSN:15K OHM,5%,0.25W	01121	CB1535
R641	321-0318-00			RES.,FXD,FILM:20K OHM,1%,0.125W	91637	MFF1816G20001F
R642	321-0352-00			RES.,FXD,FILM:45.3K OHM,1%,0.125W	91637	MFF1816G45301F
R691	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R692	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R704	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R705	315-0102-00			RES.,FXD,CMPSN:1K OHM,5%,0.25W	01121	CB1025
R736	315-0244-00			RES.,FXD,CMPSN:240K OHM,5%,0.25W	01121	CB2445
R737	315-0104-00			RES.,FXD,CMPSN:100K OHM,5%,0.25W	01121	CB1045
R748	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R749	315-0362-00			RES.,FXD,CMPSN:3.6K OHM,5%,0.25W	01121	CB3625
R751	315-0432-00			RES.,FXD,CMPSN:4.3K OHM,5%,0.25W	01121	CB4325
R752	315-0512-00			RES.,FXD,CMPSN:5.1K OHM,5%,0.25W	01121	CB5125
R753	315-0303-00			RES.,FXD,CMPSN:30K OHM,5%,0.25W	01121	CB3035
R754	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R755	311-1231-00			RES.,VAR,NONWIR:25K OHM,20%,0.50W	32997	3386F-T04-253
R756	315-0152-00			RES.,FXD,CMPSN:1.5K OHM,5%,0.25W	01121	CB1525
R757	315-0753-00			RES.,FXD,CMPSN:75K OHM,5%,0.25W	01121	CB7535
R760	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R761	315-0512-00			RES.,FXD,CMPSN:5.1K OHM,5%,0.25W	01121	CB5125
R762	315-0512-00			RES.,FXD,CMPSN:5.1K OHM,5%,0.25W	01121	CB5125
R763	315-0202-00			RES.,FXD,CMPSN:2K OHM,5%,0.25W	01121	CB2025
R764	315-0511-00			RES.,FXD,CMPSN:510 OHM,5%,0.25W	01121	CB5115
R770	315-0103-00			RES.,FXD,CMPSN:10K OHM,5%,0.25W	01121	CB1035
R771	315-0512-00			RES.,FXD,CMPSN:5.1K OHM,5%,0.25W	01121	CB5125
R772	315-0821-00			RES.,FXD,CMPSN:820 OHM,5%,0.25W	01121	CB8215
R773	315-0202-00			RES.,FXD,CMPSN:2K OHM,5%,0.25W	01121	CB2025
R774	315-0511-00			RES.,FXD,CMPSN:510 OHM,5%,0.25W	01121	CB5115

Replaceable Electrical Parts—DF1

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
R781	315-0512-00			RES.,FXD,CMPSN:5.1K OHM,5%,0.25W	01121	CB5125
R782	315-0203-00			RES.,FXD,CMPSN:20K OHM,5%,0.25W	01121	CB2035
R790	315-0244-00			RES.,FXD,CMPSN:240K OHM,5%,0.25W	01121	CB2445
R791	315-0104-00			RES.,FXD,CMPSN:100K OHM,5%,0.25W	01121	CB1045
R792	315-0511-00			RES.,FXD,CMPSN:510 OHM,5%,0.25W	01121	CB5115
S8	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S10	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S12	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S14	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S18	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S20	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S22	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S26	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S28	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S34	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S36	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S38	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S40	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S42	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S44	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S46	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S48	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S52	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S54	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
S58	263-0019-00			ACTR ASSY,PB:	80009	263-0019-00
U8	156-0572-00			MICROCIRCUIT,DI:8 BIT SERIAL IN-PRL OUT	27014	MM74C164N
U26	156-0572-00			MICROCIRCUIT,DI:8 BIT SERIAL IN-PRL OUT	27014	MM74C164N
U42	156-0572-00			MICROCIRCUIT,DI:8 BIT SERIAL IN-PRL OUT	27014	MM74C164N
U65	156-0572-00			MICROCIRCUIT,DI:8 BIT SERIAL IN-PRL OUT	27014	MM74C164N
U102	156-0469-00			MICROCIRCUIT,DI:3-LINE TO 8-LINE DECODER	01295	SN74LS138N
U110	156-0503-00			MICROCIRCUIT,DI:HEX INVERTER BUFFER	80009	156-0503-00
U132	156-0625-00			MICROCIRCUIT,DI:8 BIT PRL LOAD SHIFT RGTR	27014	MM74C165N
U138	156-0625-00			MICROCIRCUIT,DI:8 BIT PRL LOAD SHIFT RGTR	27014	MM74C165N
U152	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U156	156-0349-01			MICROCIRCUIT,DI:QUAD 2-INPUT NOR GATE	80009	156-0349-01
U158	156-0366-00			MICROCIRCUIT,LI:DUAL D-TYPE F-F	04713	MC14013CL
U162	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U172	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U182	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U216	156-0385-00			MICROCIRCUIT,DI:HEX. INVERTER	01295	SN74LS04N
U217	156-0382-00			MICROCIRCUIT,DI:QUAD 2-INPUT NAND GATE	01295	SN74LS00N
U218	156-0171-00			MICROCIRCUIT,DI:QUAD 2-INPUT OR GATE	01295	SN7432N
U222	156-0403-00			MICROCIRCUIT,DI:HEX. INV W/OPEN COLL OUTPS	01295	SN74S05N
U264	156-0426-00			MICROCIRCUIT,DI:MICROPROCESSOR 6800	04713	MC6800L
U268	156-0469-00			MICROCIRCUIT,DI:3-LINE TO 8-LINE DECODER	01295	SN74LS138N
U274	156-0716-00			MICROCIRCUIT,DI:128 X 8 BIT STATIC RAM	04713	6810A
U284	156-0899-00			MICROCIRCUIT,DI:2048 X 8 ROM,CUSTOM MASK	80009	156-0899-00
U294	156-0900-00			MICROCIRCUIT,DI:2048 X 8 ROM,CUSTOM MASK	80009	156-0900-00
U304	156-0649-00			MICROCIRCUIT,DI:3 STATE HEX. NON INVT BFR	27014	MM80C97N
U308	156-0649-00			MICROCIRCUIT,DI:3 STATE HEX. NON INVT BFR	27014	MM80C97N
U310	156-0733-00			MICROCIRCUIT,DI:DUAL MONOSTABLE MV W/ST INP	27014	DM74LS221N
U314	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U316	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
U318	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U320	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U334	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U336	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U338	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U340	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U354	156-0649-00			MICROCIRCUIT,DI:3 STATE HEX. NON INVT BFR	27014	MM80C97N
U402	156-0741-00			MICROCIRCUIT,DI:4-BIT BINARY COUNTER	80009	156-0741-00
U404	156-0387-00			MICROCIRCUIT,DI:DUAL J-K NEG EDGE TRIG	01295	SN74LS73N
U409	156-0386-00			MICROCIRCUIT,DI:TRIPLE 3-INPUT NAND GATE	01295	SN74LS10N
U412	156-0656-00			MICROCIRCUIT,DI:DECADE COUNTER	01295	SN74LS90N
U415	156-0385-00			MICROCIRCUIT,DI:HEX. INVERTER	01295	SN74LS04N
U417	156-0382-00			MICROCIRCUIT,DI:QUAD 2-INPUT NAND GATE	01295	SN74LS00N
U422	156-0785-09			MICROCIRCUIT,LI:PROM	80009	156-0785-09
U432	156-0679-00			MICROCIRCUIT,DI:4-BIT BINARY FULL ADDER	27014	DM74LS283N
U434	156-0679-00			MICROCIRCUIT,DI:4-BIT BINARY FULL ADDER	27014	DM74LS283N
U452	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U454	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U462	156-0530-00			MICROCIRCUIT,DI:SEL/MULTIPLEXE,16 PIN DIP	80009	156-0530-00
U464	156-0530-00			MICROCIRCUIT,DI:SEL/MULTIPLEXE,16 PIN DIP	80009	156-0530-00
U468	156-0509-00			MICROCIRCUIT,LI:8 BIT BIN,MULT,CURRENT OUTPUT	04713	SC20803LH
U492	156-0067-00			MICROCIRCUIT,LI:OPERATIONAL AMPLIFIER	80009	156-0067-00
U502	156-0741-00			MICROCIRCUIT,DI:4-BIT BINARY COUNTER	80009	156-0741-00
U503	156-0464-00			MICROCIRCUIT,DI:DUAL 4-INPUT NAND GATE	01295	SN74LS20N
U504	156-0741-00			MICROCIRCUIT,DI:4-BIT BINARY COUNTER	80009	156-0741-00
U522	156-0785-08			MICROCIRCUIT,DI:PROM	80009	156-0785-08
U532	156-0679-00			MICROCIRCUIT,DI:4-BIT BINARY FULL ADDER	27014	DM74LS283N
U534	156-0679-00			MICROCIRCUIT,DI:4-BIT BINARY FULL ADDER	27014	DM74LS283N
U552	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U554	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U562	156-0530-00			MICROCIRCUIT,DI:SEL/MULTIPLEXE,16 PIN DIP	80009	156-0530-00
U564	156-0530-00			MICROCIRCUIT,DI:SEL/MULTIPLEXE,16 PIN DIP	80009	156-0530-00
U568	156-0509-00			MICROCIRCUIT,LI:8 BIT BIN,MULT,CURRENT OUTPUT	04713	SC20803LH
U604	156-0733-00			MICROCIRCUIT,DI:DUAL MONOSTABLE MV WITH ST INP	27014	DM74LS221N
U614	156-0386-00			MICROCIRCUIT,DI:TRIPLE 3-INPUT NAND GATE	01295	SN74LS10N
U624	156-0733-00			MICROCIRCUIT,DI:DUAL MONOSTABLE MV WITH ST INP	27014	DM74LS221N
U632	156-0412-00			MICROCIRCUIT,DI:4-BIT BIN UP/DOWN COUNTER	01295	SN74LS193N
U634	156-0412-00			MICROCIRCUIT,DI:4-BIT BIN UP/DOWN COUNTER	01295	SN74LS193N
U636	156-0412-00			MICROCIRCUIT,DI:4-BIT BIN UP/DOWN COUNTER	01295	SN74LS193N
U638	156-0388-00			MICROCIRCUIT,DI:DUAL D-TYPE FLIP-FLOP	01295	SN74LS74N
U640	156-0402-00			MICROCIRCUIT,DI:TIMER	18324	NE555V
U641	156-0469-00			MICROCIRCUIT,DI:3-LINE TO 8-LINE DECODER	01295	SN74LS138N
U642	156-0547-00			MICROCIRCUIT,DI:QUAD TOW-INPUT MULTIPLEXER	27014	MM74C157N
U644	156-0547-00			MICROCIRCUIT,DI:QUAD TOW-INPUT MULTIPLEXER	27014	MM74C157N
U646	156-0547-00			MICROCIRCUIT,DI:QUAD TOW-INPUT MULTIPLEXER	27014	MM74C157N
U648	156-0387-00			MICROCIRCUIT,DI:DUAL J-K NEG EDGE TRIG	01295	SN74LS73N
U652	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U654	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U656	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U658	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U662	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U664	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U666	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102


Replaceable Electrical Parts—DF1

Ckt No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Name & Description	Mfr Code	Mfr Part Number
U668	156-0291-00			MICROCIRCUIT,DI:1024 BIT X STATIC ROM	34649	2102
U674	156-0391-00			MICROCIRCUIT,DI:HEX LATCH WITH CLEAR	01295	SN74LS174N
U676	156-0388-00			MICROCIRCUIT,DI:DUAL D-TYPE FLIP-FLOP	01295	SN74LS74N
U684	156-0882-00			MICROCIRCUIT,DI:ROM CHAR GEN	80009	156-0882-00
U694	156-0073-00			MICROCIRCUIT,DI:SGL 10MHZ SHIFT REG	01295	SN7496N
U704	156-0385-00			MICROCIRCUIT,DI:HEX. INVERTER	01295	SN74LS04N
U714	156-0388-00			MICROCIRCUIT,DI:DUAL D-TYPE FLIP-FLOP	01295	SN74LS74N
U724	156-0382-00			MICROCIRCUIT,DI:QUAD 2-INPUT NAND GATE	01295	SN74LS00N
U735	156-0574-00			MICROCIRCUIT,DI:TRI-STATE QUAD D F-F	27014	MM74C173N
U738	156-0387-00			MICROCIRCUIT,DI:DUAL J-K NEG EDGE TRIG	01295	SN74LS73N
U746	156-0382-00			MICROCIRCUIT,DI:QUAD 2-INPUT NAND GATE	01295	SN74LS00N
U748	156-0733-00			MICROCIRCUIT,DI:DUAL MONOSTABLE MV WITH ST INP	27014	DM74LS221N
U752	156-0386-00			MICROCIRCUIT,DI:TRIPLE 3-INPUT NAND GATE	01295	SN74LS10N
U756	156-0383-00			MICROCIRCUIT,DI:QUAD 2-INPUT NOR GATE	01295	SN74LS02N
VR62	152-0481-00			SEMICONV DEVICE:ZENER,1W,5.1V,5%	04713	1N3826A
Y704	158-0056-00			XTAL UNIT,QTZ:4 MHZ,0.003%,SERIES RESN	80009	158-0056-00

INSTRUMENT OPTIONS

No options were available for this instrument at the time of this printing.

Information on any subsequent options may be found in the CHANGE INFORMATION section in the back of this manual.

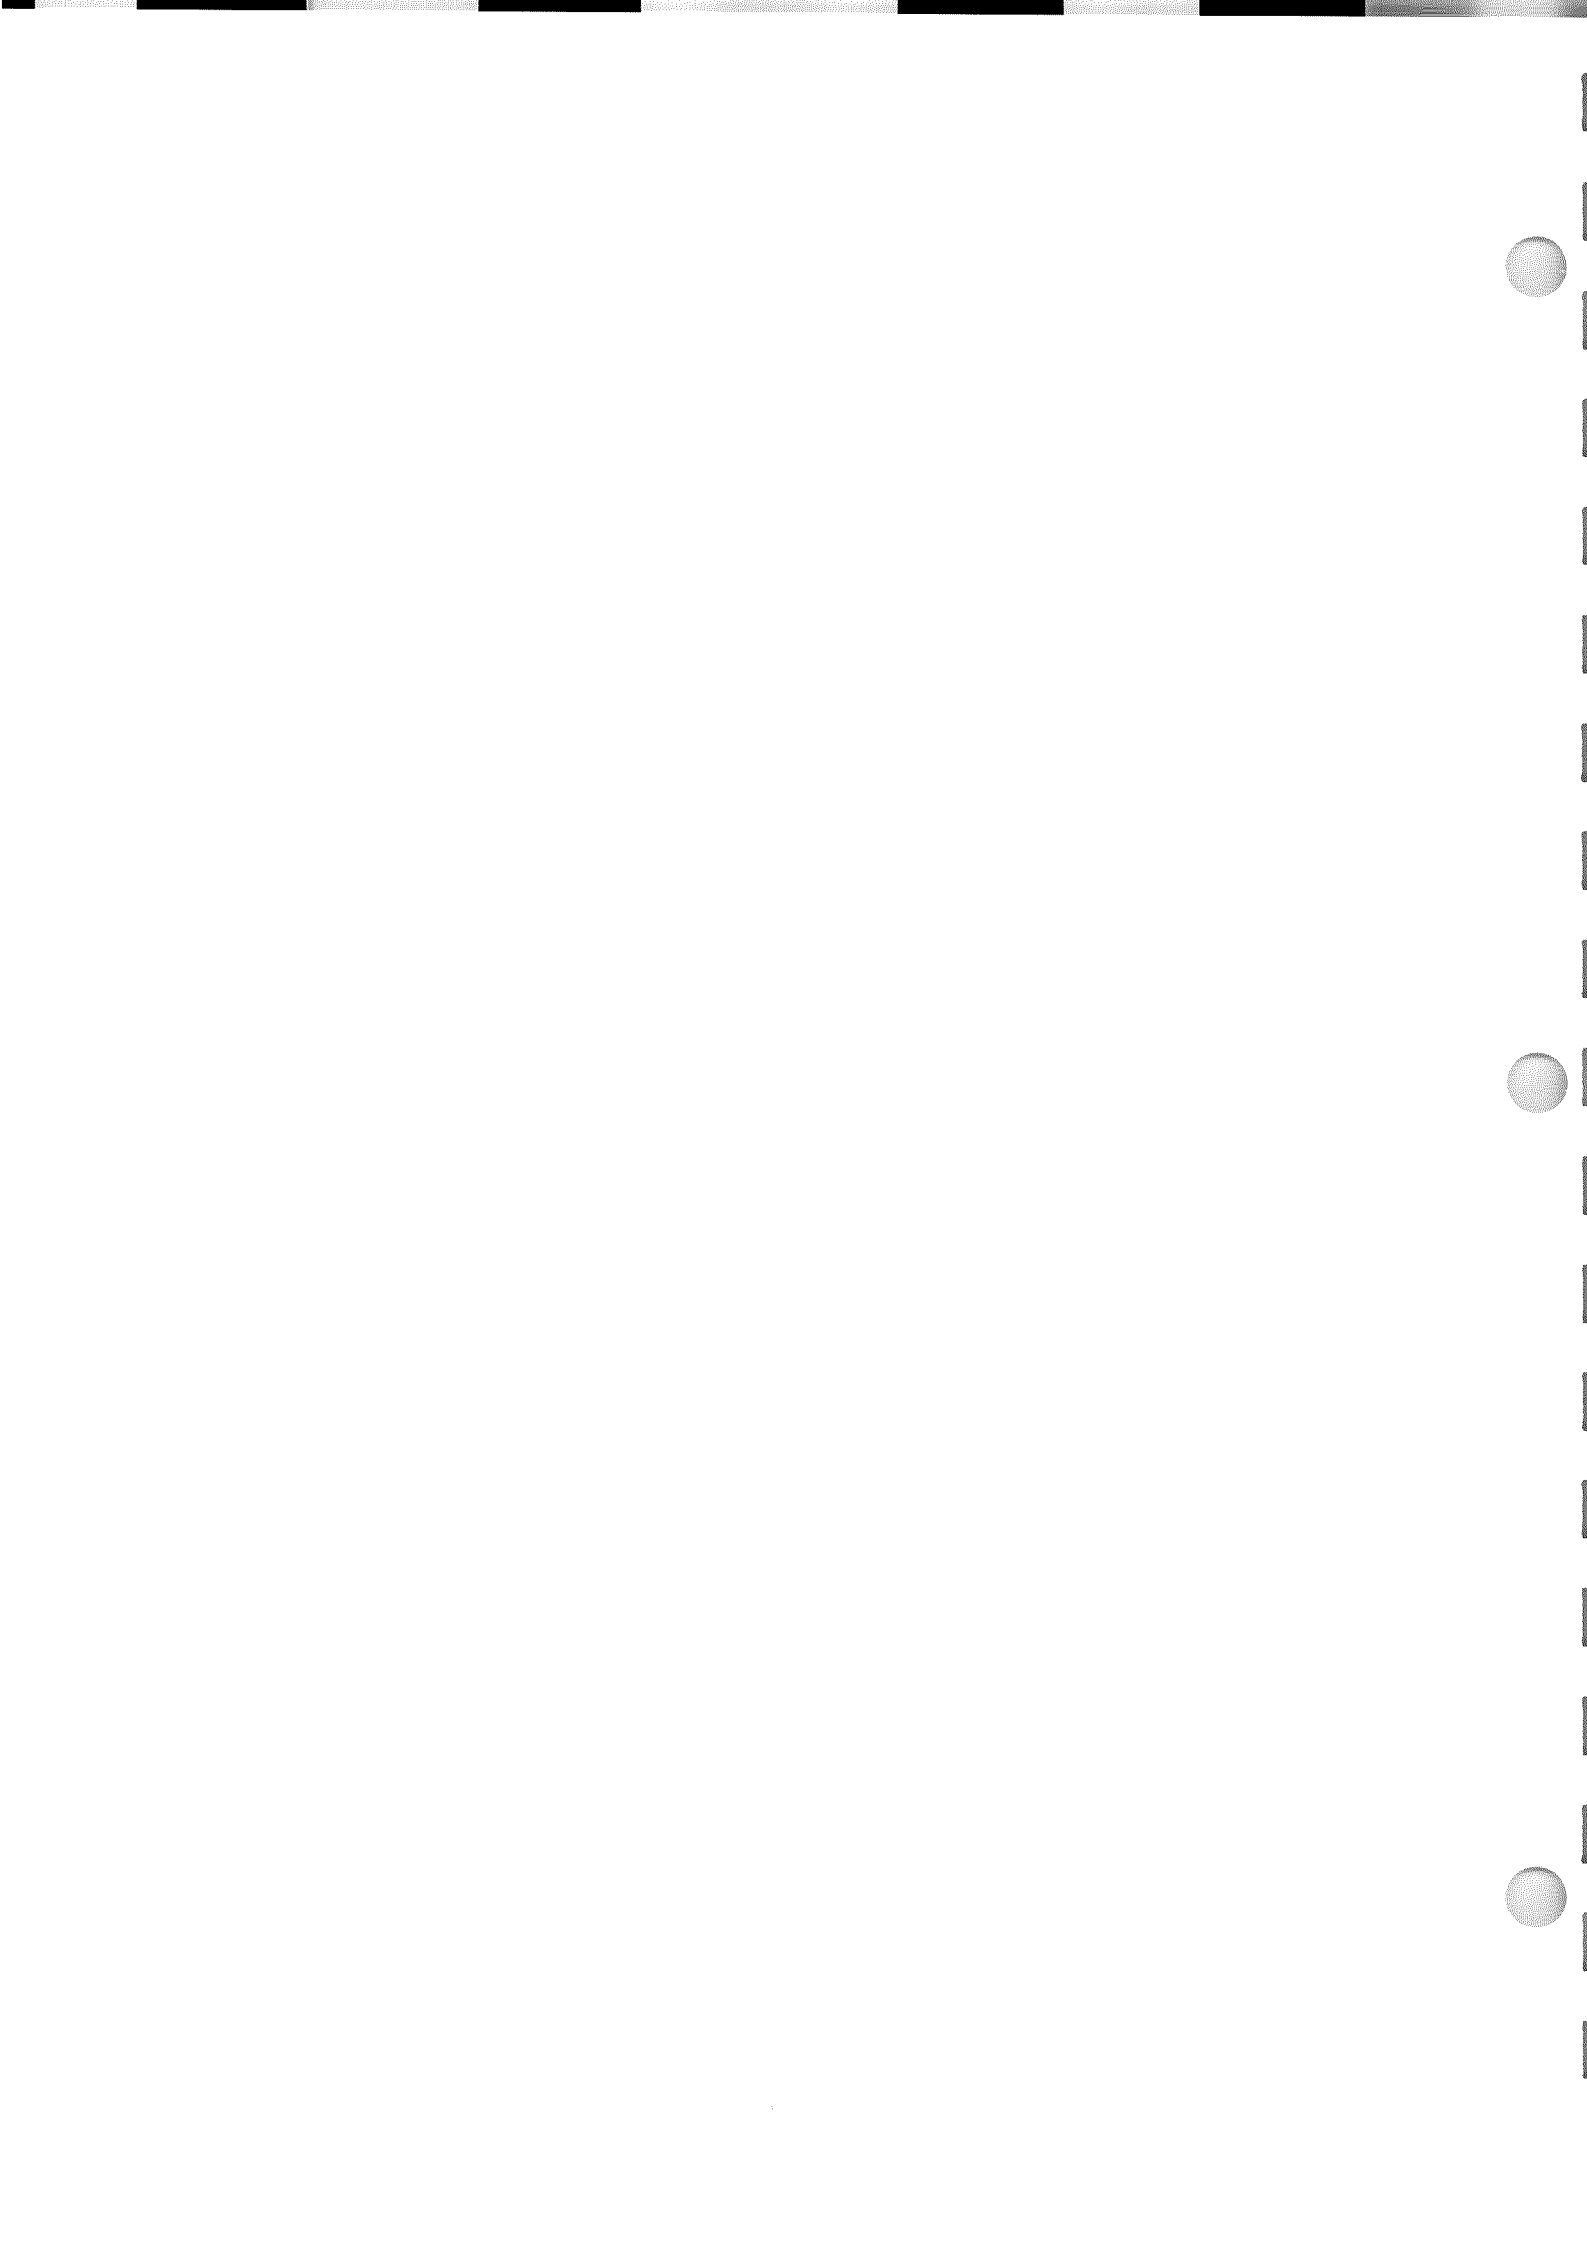

DIAGRAMS AND CIRCUIT BOARD ILLUSTRATIONS

Symbols and Reference Designators

Electrical components shown on the diagrams are in the following units unless noted otherwise:

Capacitors = Values one or greater are in picofarads (pF).
Values less than one are in microfarads (μ s).

Resistors = Ohms (Ω).


Symbols used on the diagrams are based on ANSI Standard Y32.2-1975.



Logic symbology is based on ANSI Y32.14-1973 in terms of positive logic. Logic symbols depict the logic function performed and may differ from the manufacturer's data.

The following prefix letters are used as reference designators to identify components or assemblies on the diagrams.

A	Assembly, separable or repairable (circuit board, etc.)	H	Heat dissipating device (heat sink, heat radiator, etc.)	RT	Thermistor
AT	Attenuator, fixed or variable	HR	Heater	S	Switch
B	Motor	HY	Hybrid circuit	T	Transformer
BT	Battery	J	Connector, stationary portion	TC	Thermocouple
C	Capacitor, fixed or variable	K	Relay	TP	Test point
CB	Circuit breaker	L	Inductor, fixed or variable	U	Assembly, inseparable or non-repairable (integrated circuit, etc.)
CR	Diode, signal or rectifier	LR	Inductor/resistor combination	V	Electron tube
DL	Delay line	M	Meter	VR	Voltage regulator (zener diode, etc.)
DS	Indicating device (lamp)	P	Connector, movable portion	Y	Crystal
E	Spark Gap	Q	Transistor or silicon-controlled rectifier	Z	Phase shifter
F	Fuse	R	Resistor, fixed or variable		
FL	Filter				


The following special symbols are used on the diagrams:

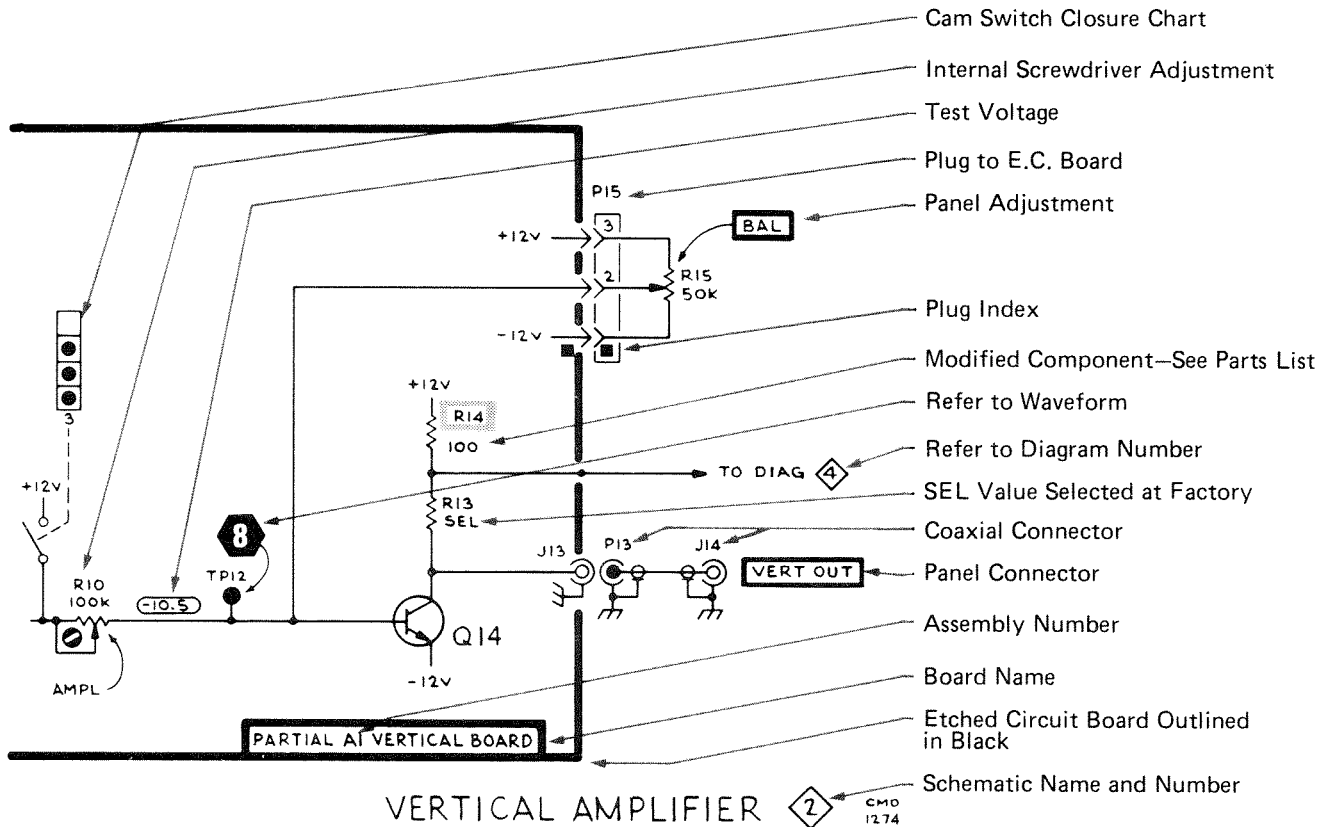




DARLINGTON

PLASTIC-CASED TRANSISTORS








METAL CASE TRANSISTOR

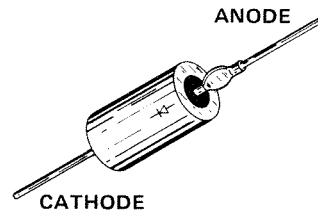


CATHODE

DIODE

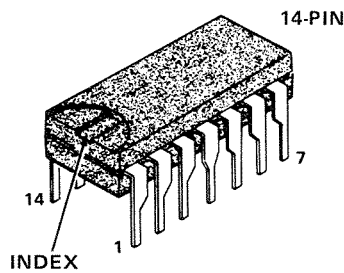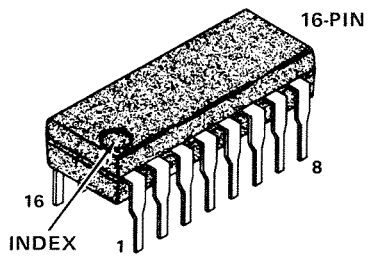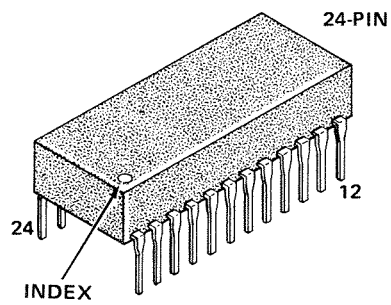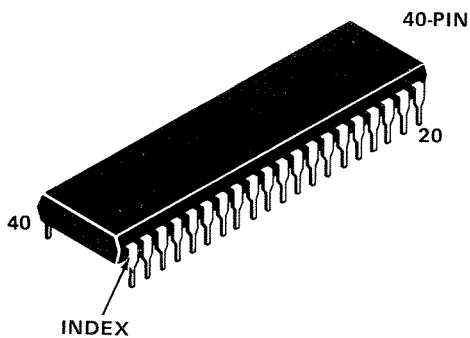

INTEGRATED CIRCUITS


Figure 8-1. Semiconductor lead configurations.

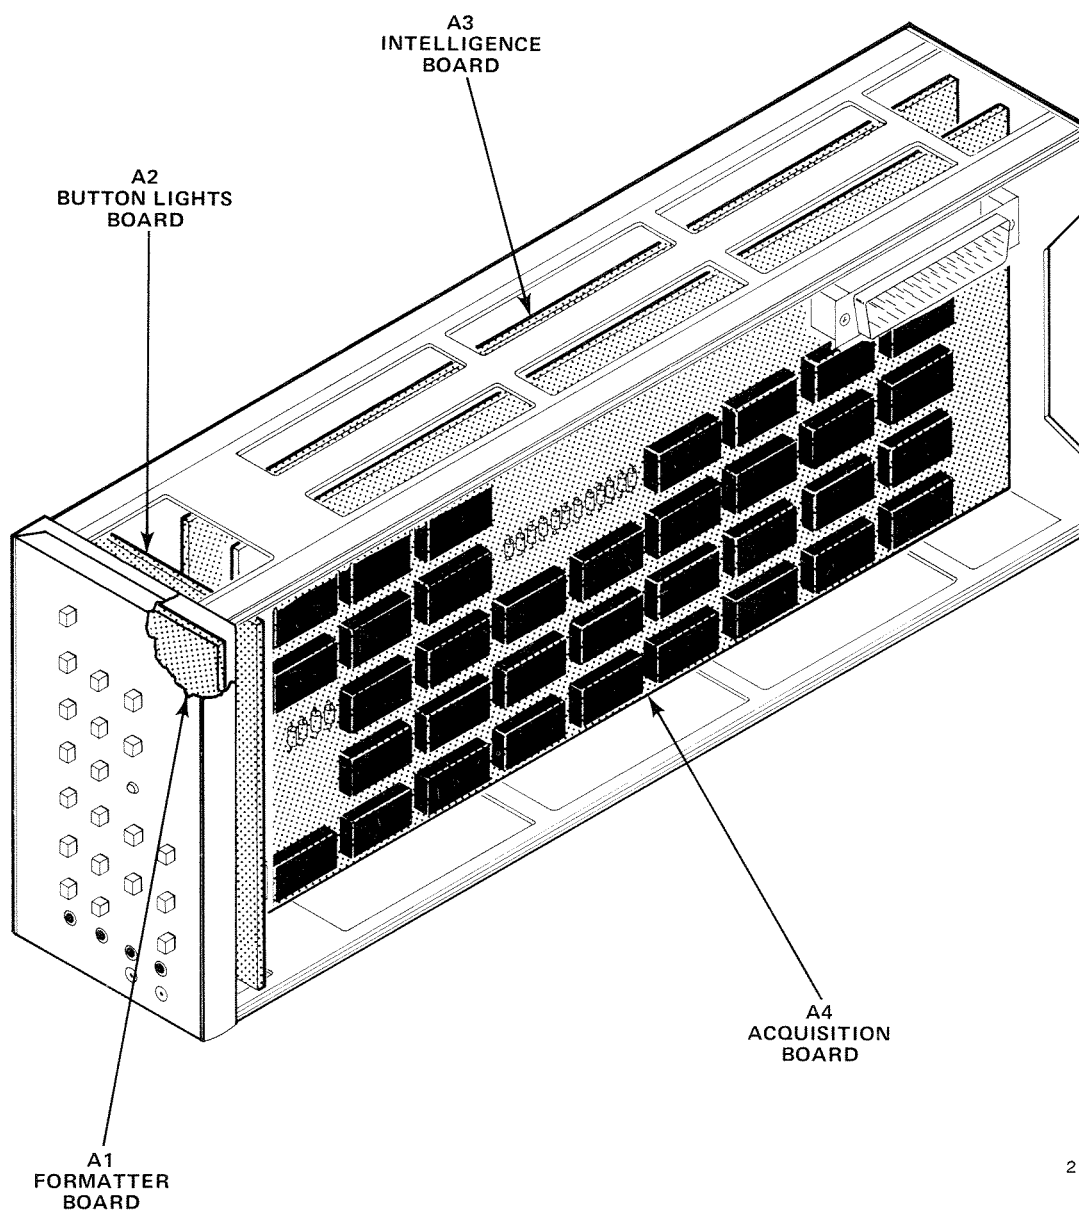

2150-132

Figure 8-2. Circuit board locations.

DF1 TROUBLESHOOTING CHART

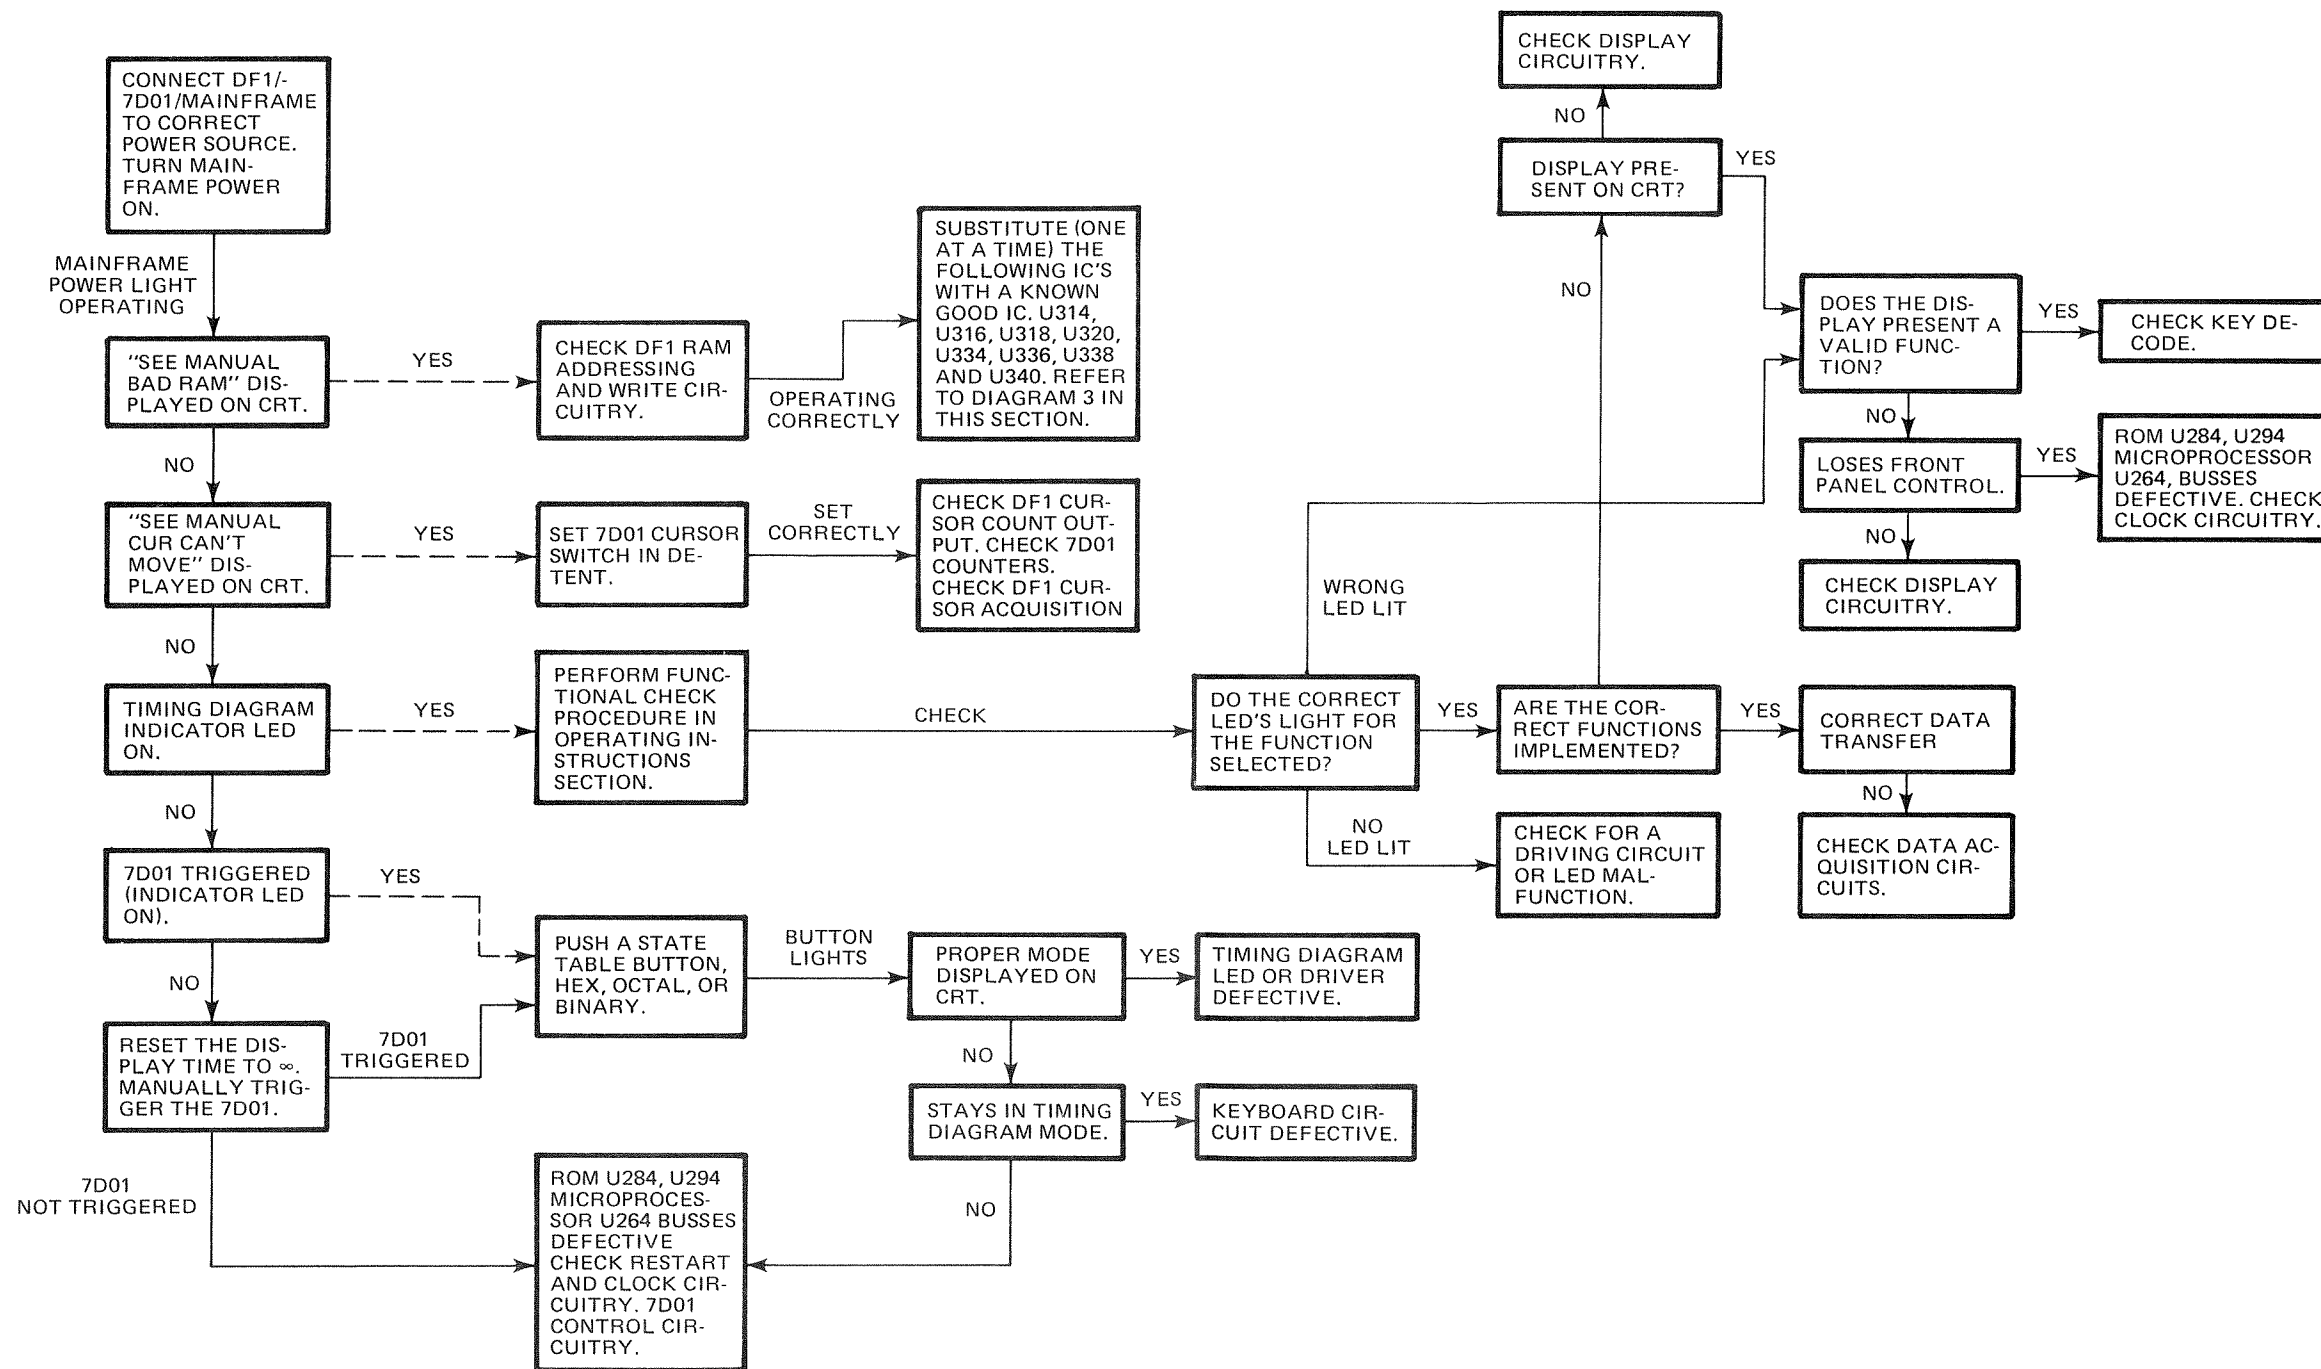

DF1 TROUBLESHOOTING CHART

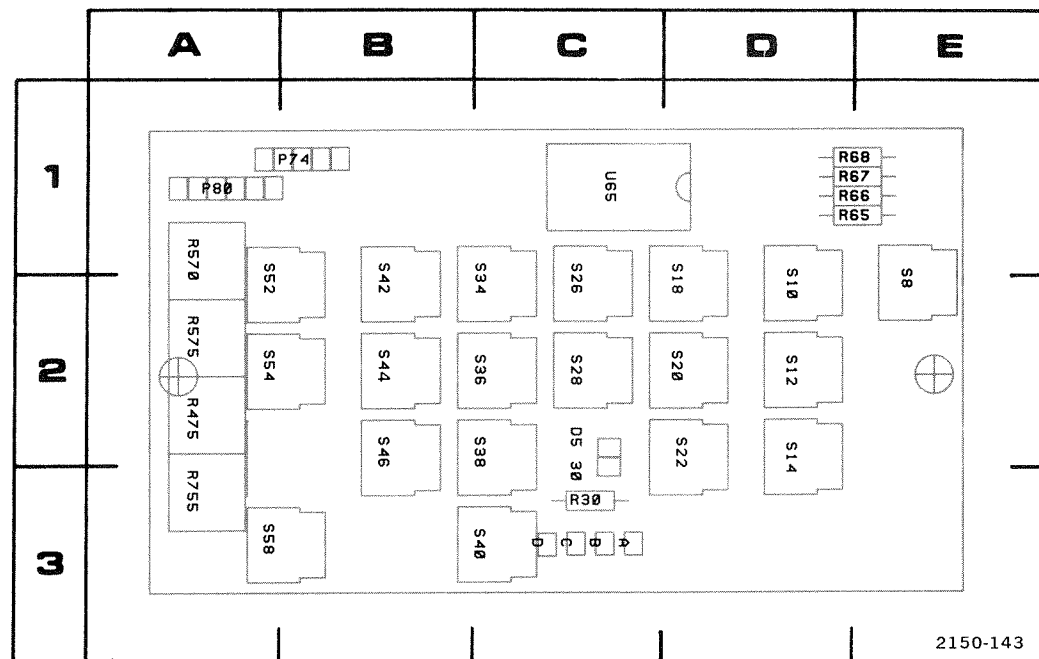


Figure 8-3. A1—Formatter Keyboard circuit board locations as viewed from front of instrument.

CKT NO	GRID COORD	CKT NO	GRID COORD
DS30	2C	S18	2D
P74	1B	S20	2D
P80	1A	S22	2D
		S26	2C
R30	3C	S28	2C
R65	1D	S34	2C
R66	1D	S36	2C
R67	1D	S38	2C
R68	1D	S40	3C
R475	2A	S42	2B
R570	1A	S44	2B
R575	2A	S46	2B
R755	3A	S48	2B
		S52	2A
S8	2E	S54	2A
S10	2D	S58	3A
S12	2D		
S14	2D	U65	1C


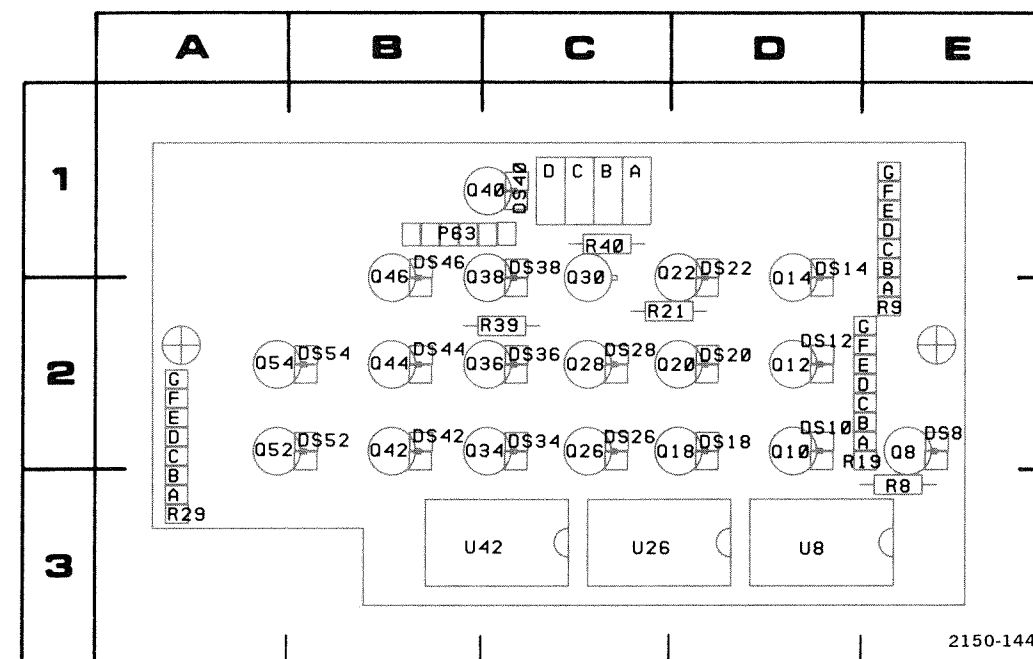


Figure 8-4. A2—Button Lights circuit board component locations as viewed from the component side of the board.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
DS8	2E	P63	1B	Q46	1B
DS10	2D			Q52	2A
DS12	2D	Q8	2E	Q54	2A
DS14	1D	Q10	2D		
DS18	2D	Q12	2D	R8	3E
DS20	2D	Q14	1D	R9	2E
DS22	1D	Q18	2C	R19	2E
DS26	2C	Q20	2C	R21	2C
DS28	2C	Q22	1D	R29	3A
DS34	2C	Q26	2C	R39	2C
DS36	2C	Q28	2C	R40	1C
DS38	1C	Q30	1C		
DS40	1C	Q34	2B	U8	3D
DS42	2B	Q36	2B	U26	3C
DS44	2B	Q38	1B	U42	3C
DS46	1B	Q40	1C		
DS52	2B	Q42	2B		
DS54	2B	Q44	2B		

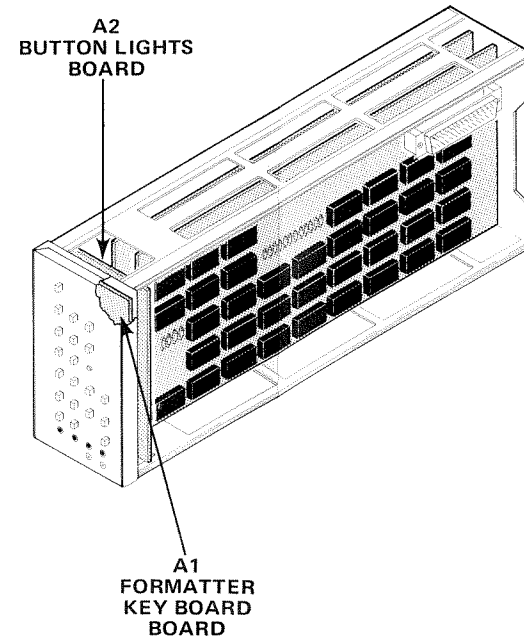



J. I. C.
B1 P2

SEE PARTS LIST FOR
SEMICONDUCTOR TYPES.

FRONT PANEL


DFI

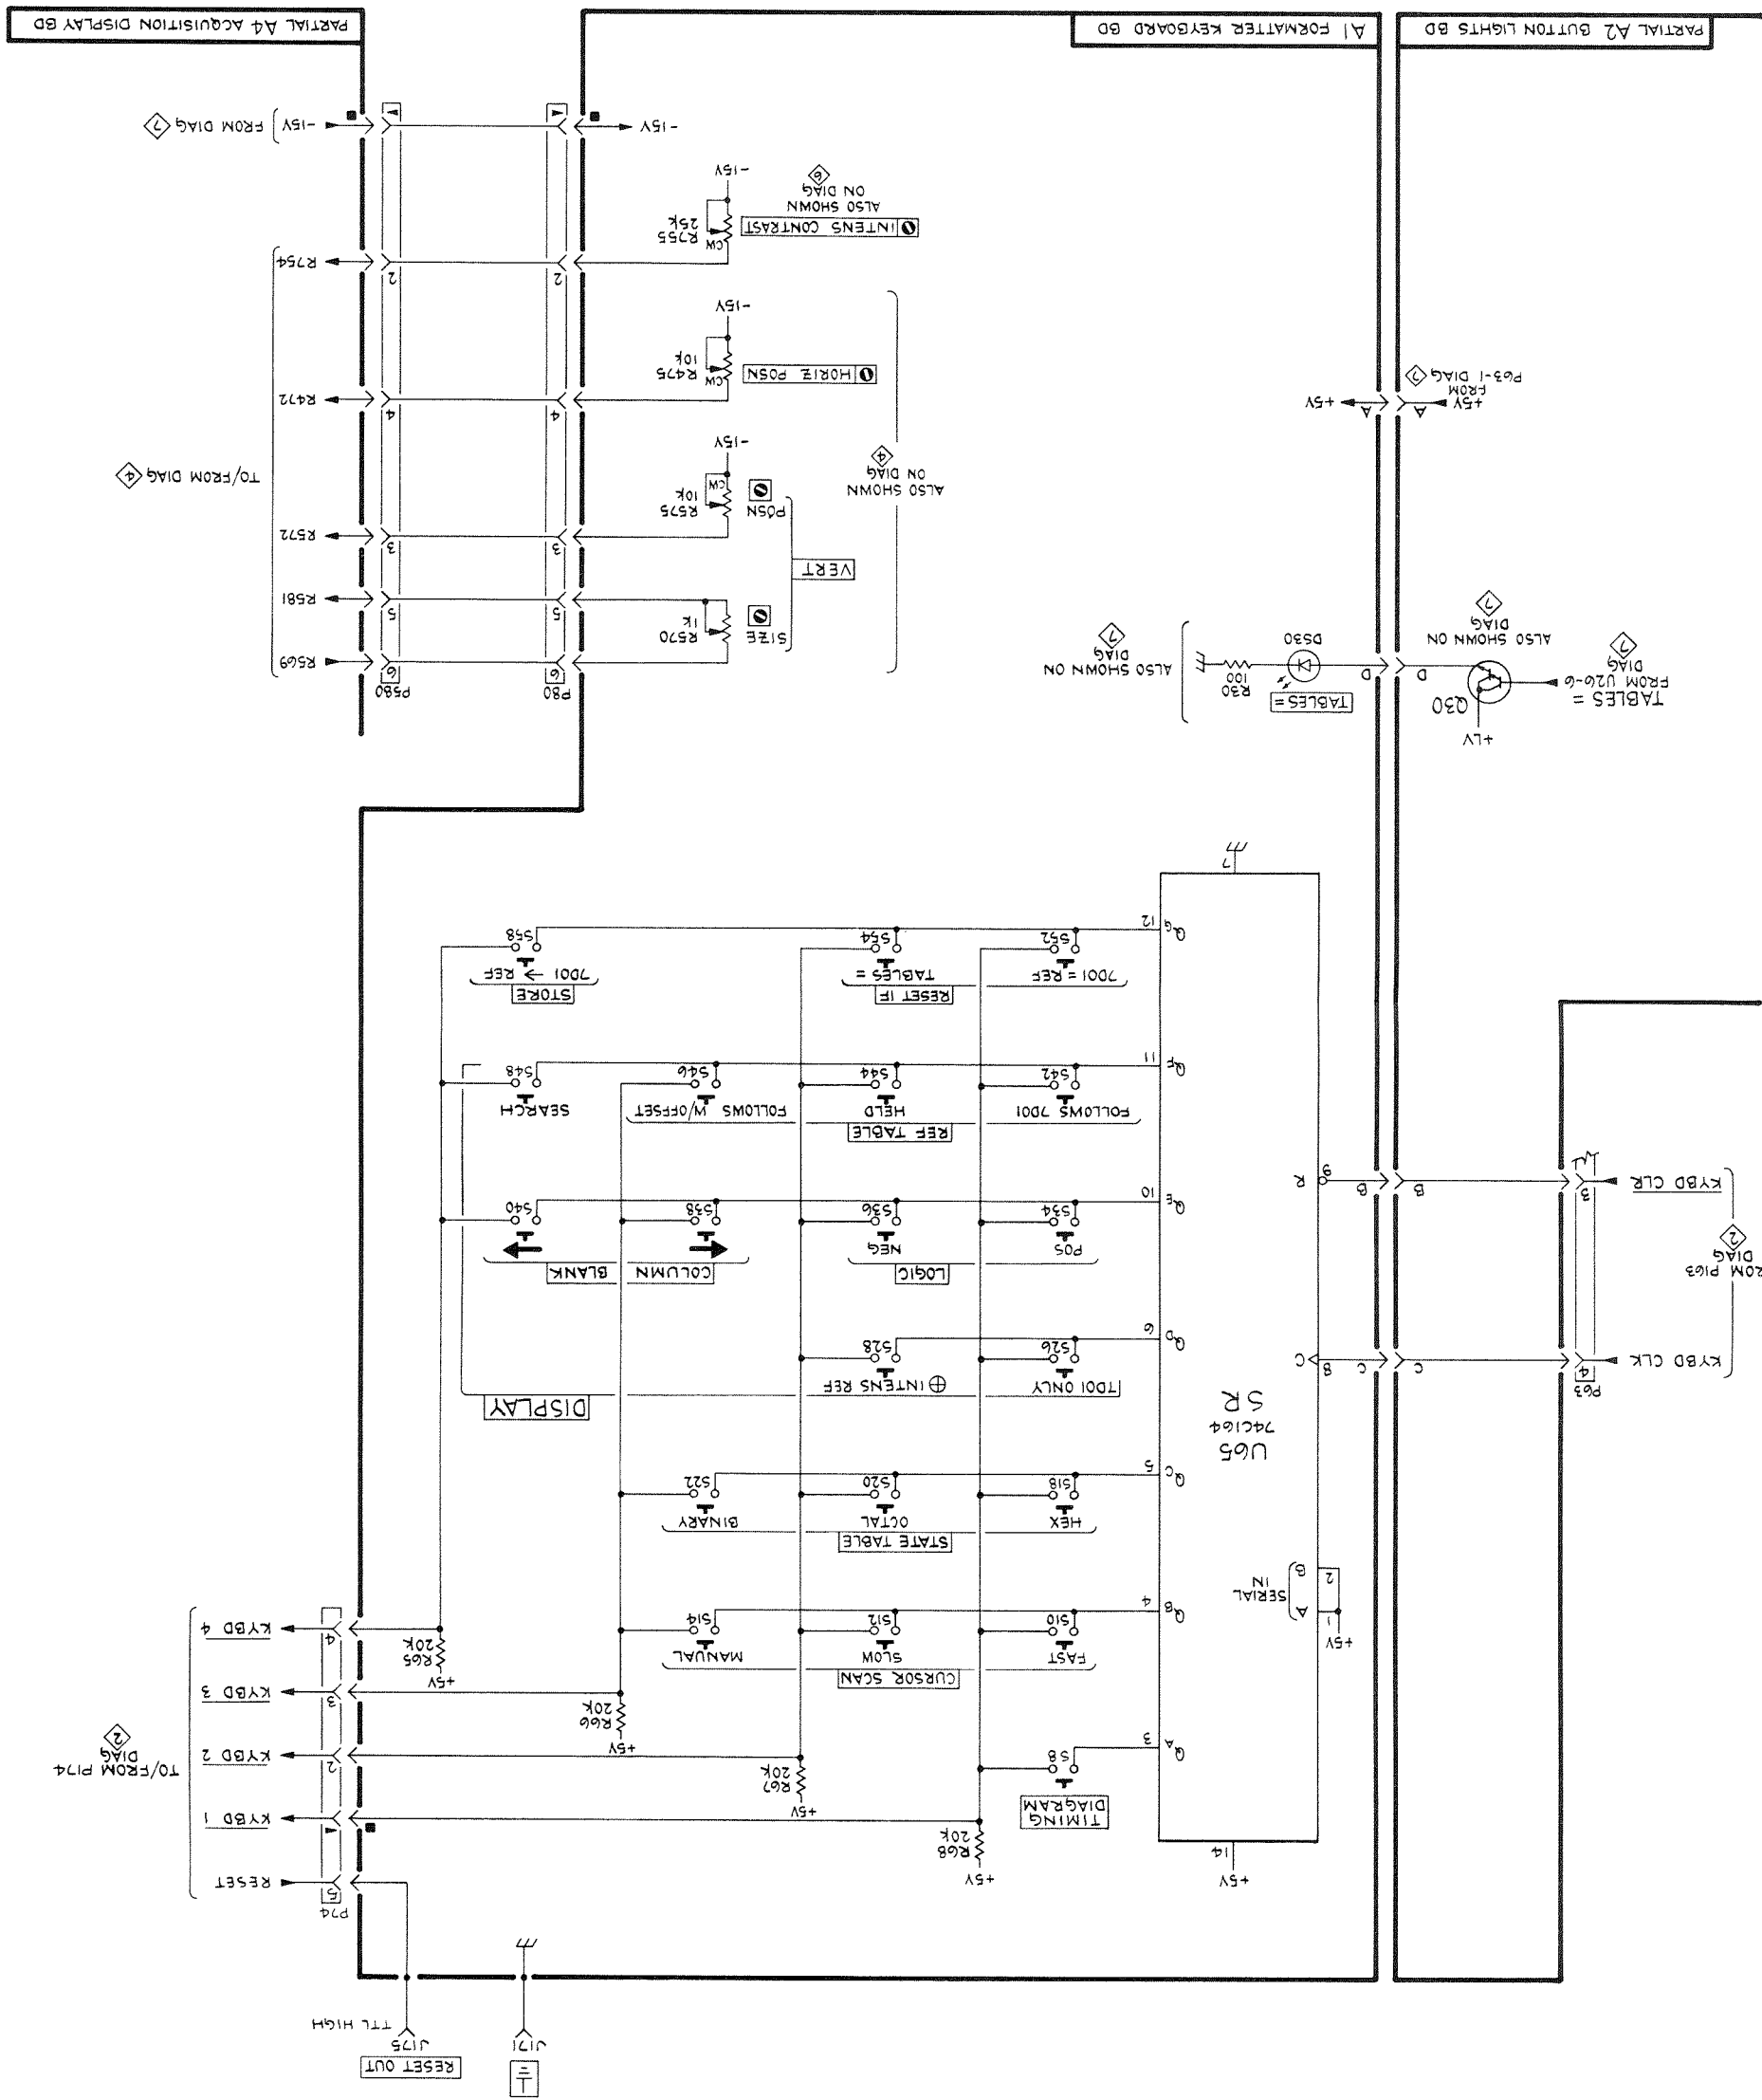


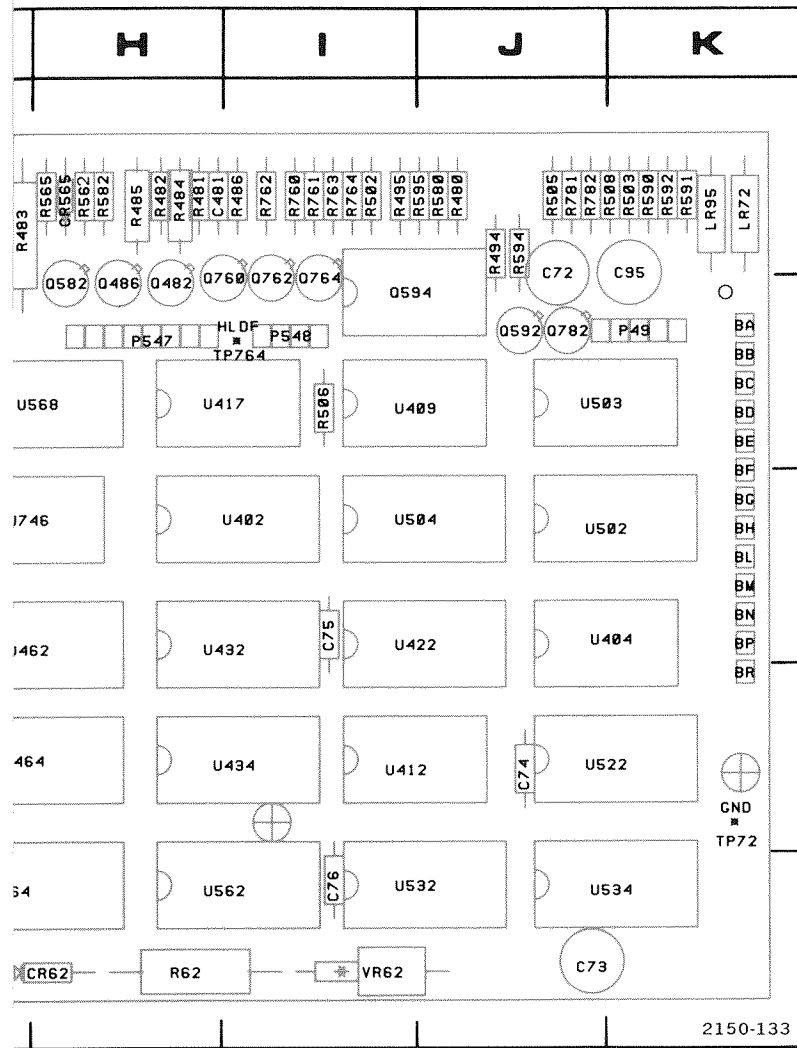

tions.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C72	1J	Q141	5C	R503	1K	U110	4C
C73	5J	Q151	5A	R505	1J	U132	5E
C74	4J	Q184	5E	R506	2I	U138	5G
C75	3I	Q188	5E	R508	1K	U152	3B
C76	5I	Q202	5C	R562	1H	U156	3D
C77	5G	Q206	5C	R563	2F	U158	4D
C78	4F	Q472	2F	R564	2G	U162	3B
C79	3E	Q482	2H	R565	1H	U172	4A
C93	1D	Q486	2H	R566	1G	U182	4B
C95	1K	Q572	2G	R567	2F	U402	3I
C96	4E	Q582	2H	R569	2F	U404	3K
C97	3D	Q586	2G	R571	1G	U409	2I
C98	3C	Q592	2I	R572	2G	U412	4I
C99	1C	Q594	2I	R580	1J	U415	3E
C187	5E	Q752	1E	R581	1G	U417	2I
C206	5B	Q754	2E	R582	1H	U422	3I
C467	2E	Q756	1C	R583	1G	U432	3I
C468	2F	Q760	2I	R584	1G	U434	4I
C470	2E	Q762	2I	R585	2F	U452	3E
C472	2F	Q764	2I	R586	1G	U454	3E
C481	1H	Q770	2D	R590	1K	U462	3G
C492	2E	Q772	2E	R591	1K	U464	4H
C493	2F	Q774	2D	R592	1K	U468	2F
C494	1F	Q782	2I	R594	1J	U492	2D
C567	2F	Q792	2E	R595	1J	U502	3K
C568	2F	Q796	2E	R704	1B	U503	2I
C570	2F			R705	1B	U504	3I
C572	2G	R62	5H	R736	2C	U522	4K
C581	1G	R141	5D	R737	1E	U532	5I
C583	1G	R142	5C	R748	1A	U534	5J
C704	1B	R150	3B	R749	1A	U552	4G
C705	1B	R151	5A	R751	1D	U554	4E
C748	1A	R152	5A	R752	1E	U562	5I
C749	1A	R156	5D	R753	1E	U564	5G
		R184	5E	R754	2F	U568	2H
CR62	5H	R187	5E	R756	1C	U704	2B
CR151	3B	R188	5D	R757	1C	U714	2C
CR152	3A	R201	5B	R760	1I	U724	3E
CR471	2F	R202	3B	R761	1I	U735	3D
CR564	2G	R203	5C	R762	1I	U738	3D
CR565	1H	R204	5B	R763	1I	U746	3G
CR571	1F	R205	5B	R764	1I	U748	2B
		R206	3B	R770	1D	U752	2C
L73	1E	R463	2E	R771	1D	U756	2B
L704	1B	R467	2E	R772	1D		
		R469	2E	R773	1D	VR62	5I
LR72	1K	R470	1E	R774	1D		
LR95	1K	R471	1F	R781	1J	Y704	1A
		R472	2F	R790	1C		
P49	2K	R480	1J	R791	1D		
P141	5E	R481	1H	R792	1E		
P142	5D	R482	1H				
P145	3D	R483	1G	TP70	3A		
P163	5C	R484	1H	TP72	4K		
P174	5B	R485	1H	TP492	2E		
P547	2H	R486	1I	TP704	3E		
P548	2I	R491	2E	TP748	2A		
P580	1F	R492	2E	TP764	2I		
P746	2D	R494	1J	TP774	4C		
P752	1B	R495	1I				
P754	1B	R502	1I	U102	2B		

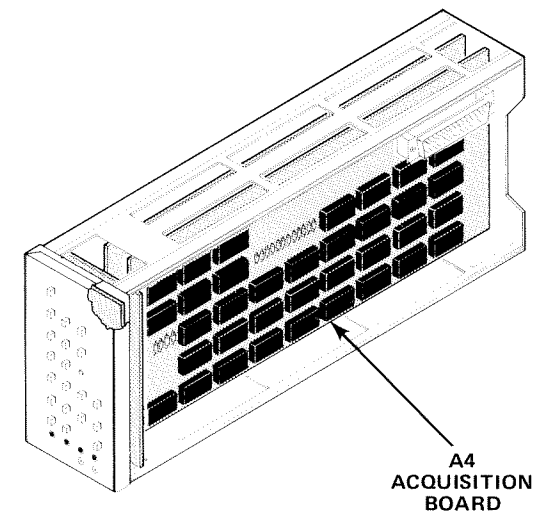

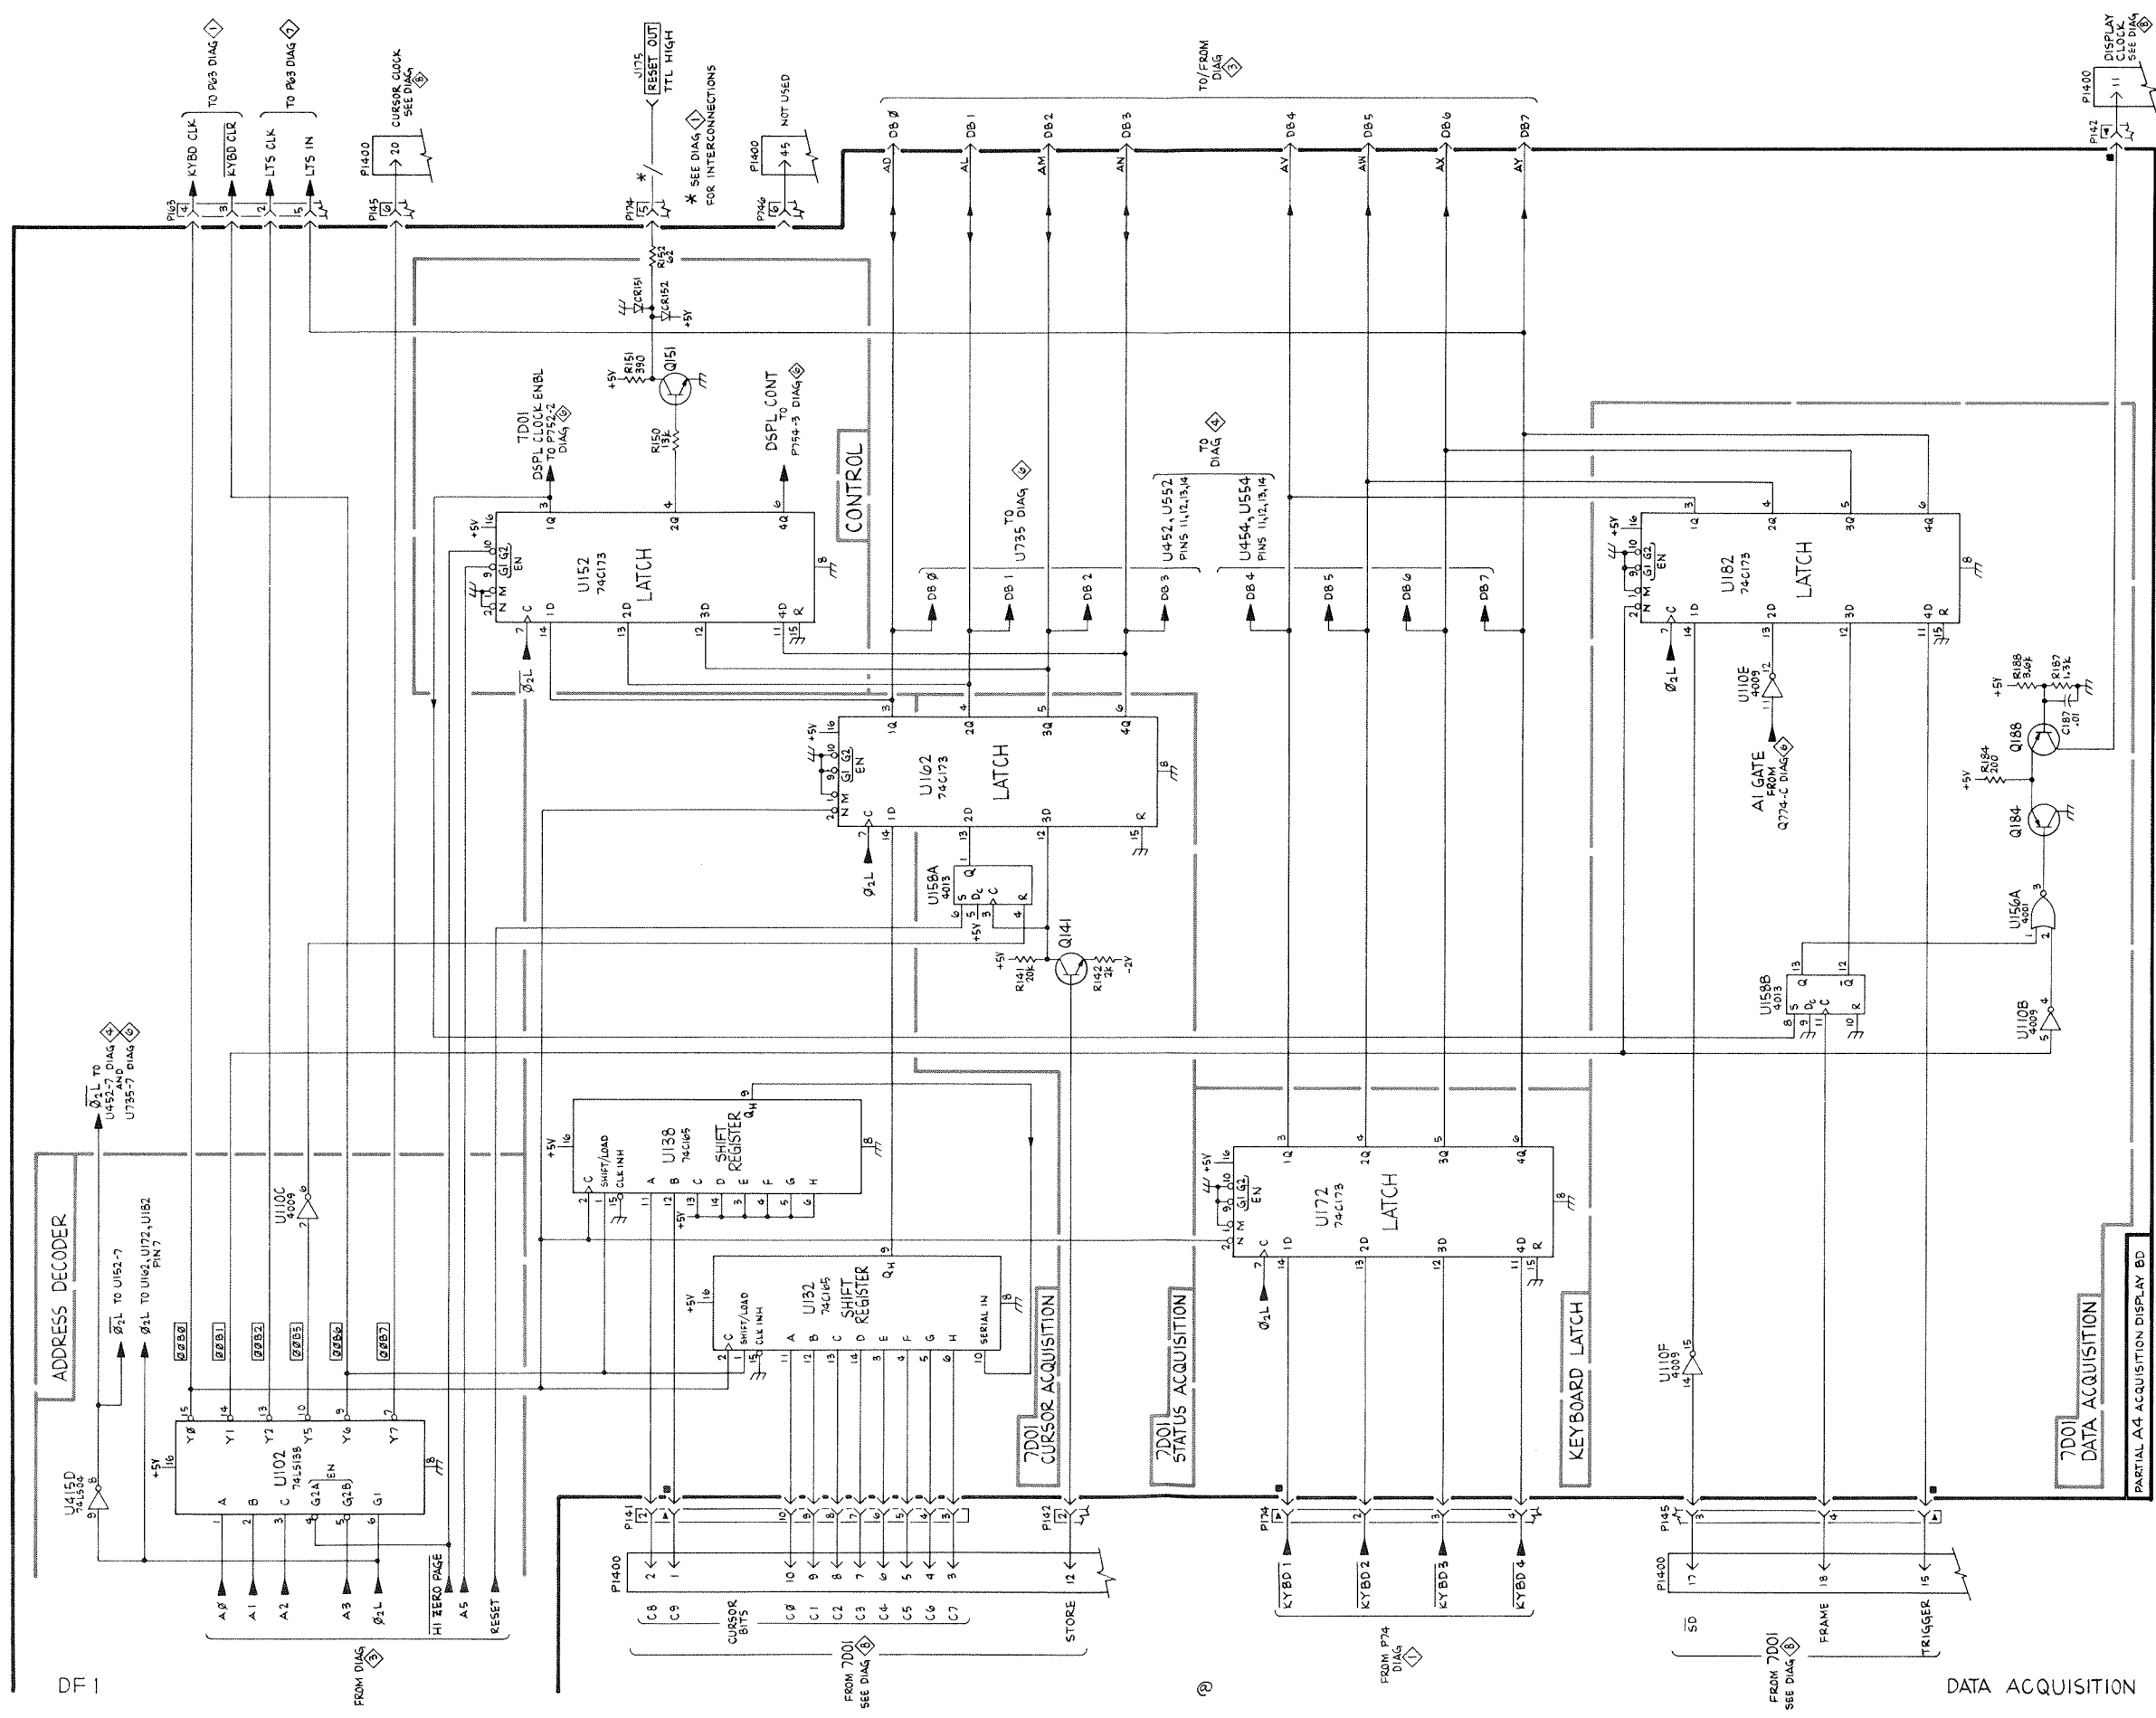

DF 1

DATA ACQUISITION

TYPE	V _{CC} (V _{DC})	I _{GN} D
74LS04	14	7
4001	14	7
4005	14	7
4013	14	7

SEE PARTS LIST FOR SEMICONDUCTOR TYPES

L.I.C.
P1 P2

2



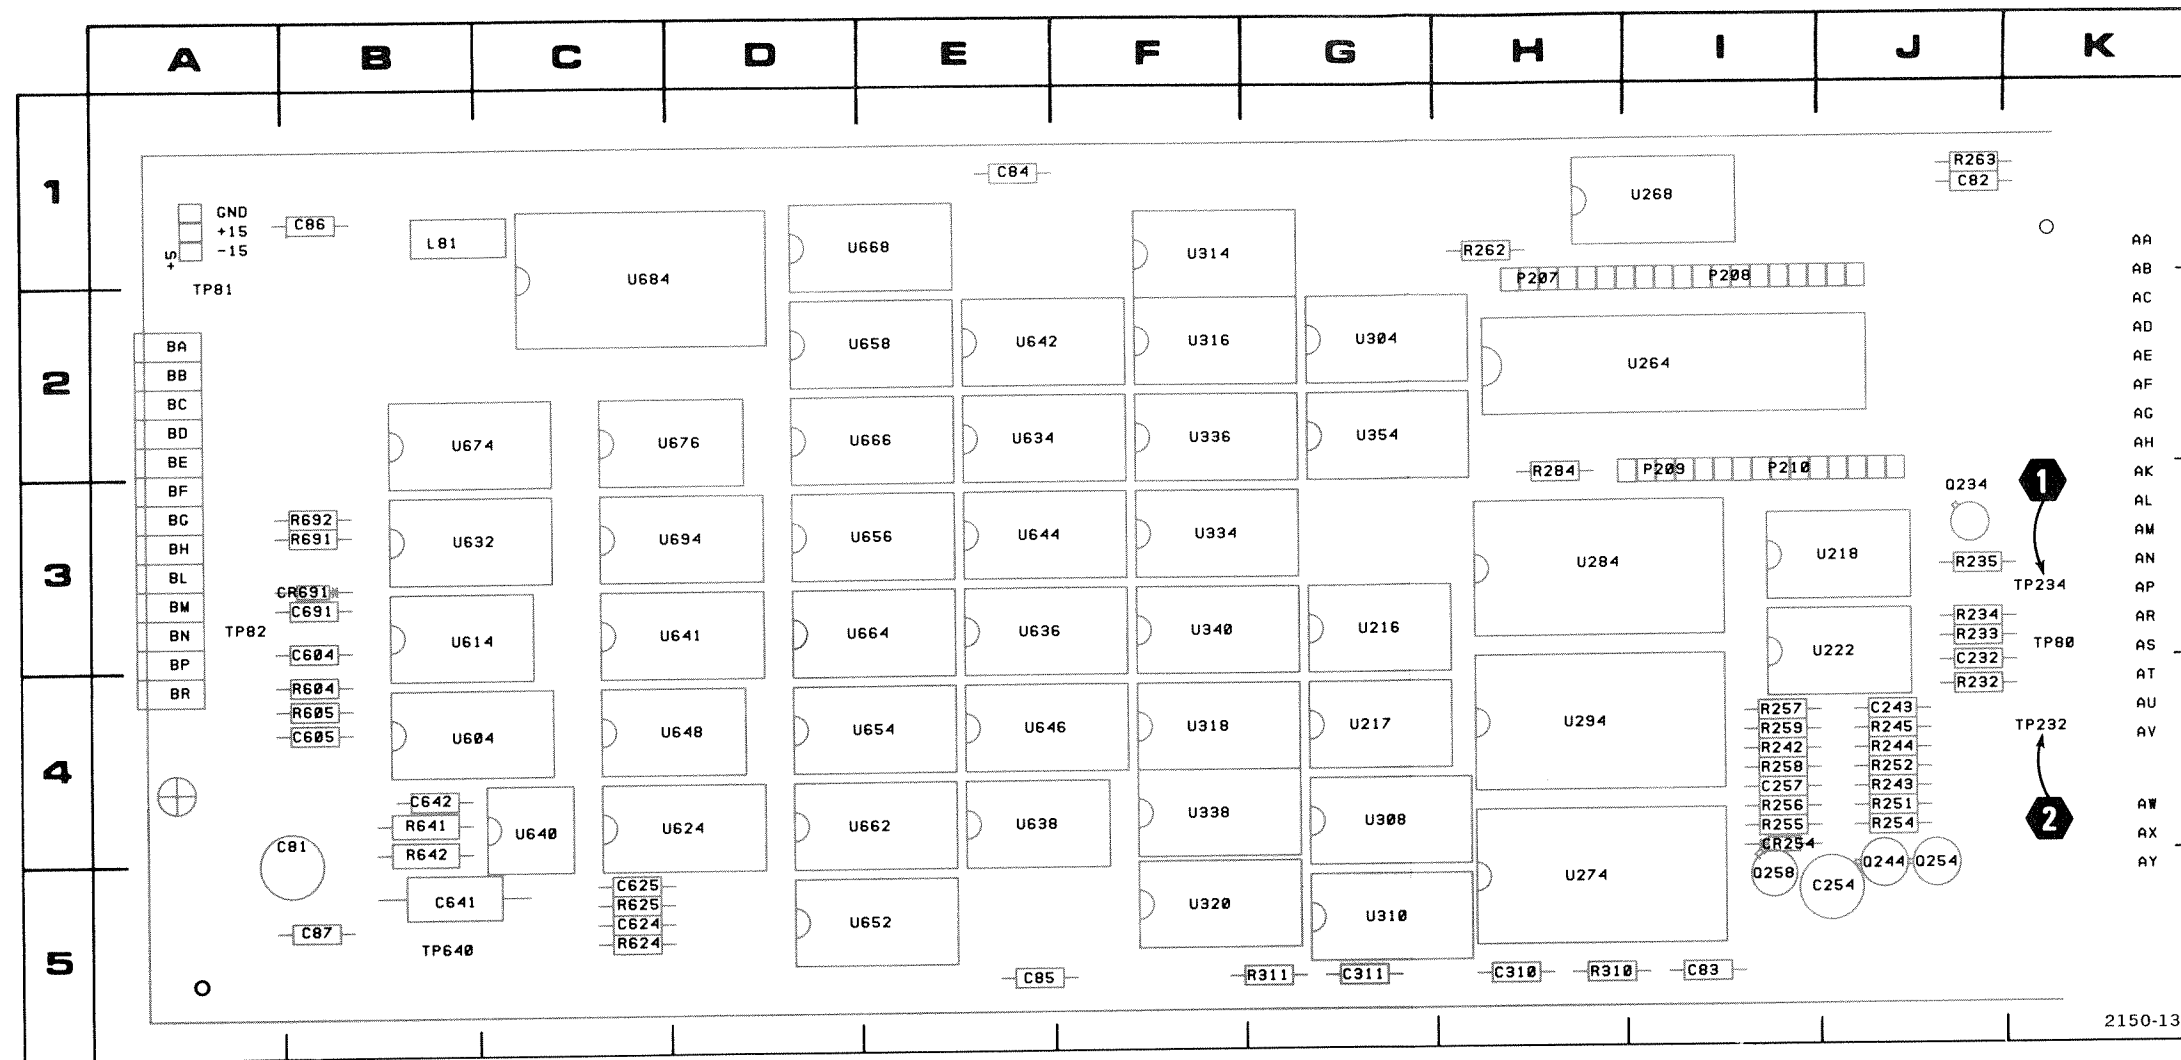


Figure 8-6. A3-Intelligence circuit board component locations.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C81	4B	R604	4B	U668	1E
C82	1J	R605	4B	U674	2B
C83	5I	R624	5C	U676	2D
C84	1E	R625	5C	U684	1C
C85	5E	R641	4B	U694	3D
C86	1B	R642	4B		
C87	5B	R691	3B	VR687	2B
C232	3J	R692	3B		
C243	4J				
C254	5J	TP80	3K		
C257	4I	TP81	1A		
C310	5H	TP82	3A		
C311	5G	TP232	4K		
C604	3B	TP234	3K		
C605	4B	TP640	5B		
C624	5C				
C625	5C	U216	3G		
C641	5B	U217	4G		
C642	4B	U218	3J		
C691	3B	U222	3J		
		U264	2I		
CR254	4I	U268	1I		
CR691	3B	U274	5H		
		U284	3H		
		U294	4H		
		U304	2G		
		U308	4G		
		U310	5G		
		U314	1F		
		U316	2F		
		U318	4F		
		U320	5F		
		U334	3F		
		U336	2F		
		U338	4F		
		U340	3F		
		U354	2G		
		U604	4C		
		U614	3C		
		U624	4D		
		U632	3C		
		U634	2E		
		U636	3E		
		U638	4E		
		U640	4C		
		U641	3D		
		U642	2E		
		U644	3E		
		U646	4E		
		U648	4D		
		U652	5E		
		U654	4E		
		U656	3E		
		U658	2E		
		U662	4E		
		U664	3E		
		U666	2E		

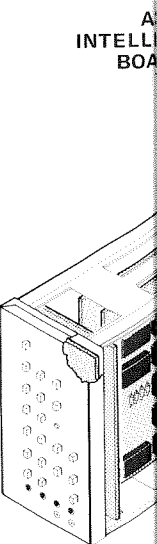

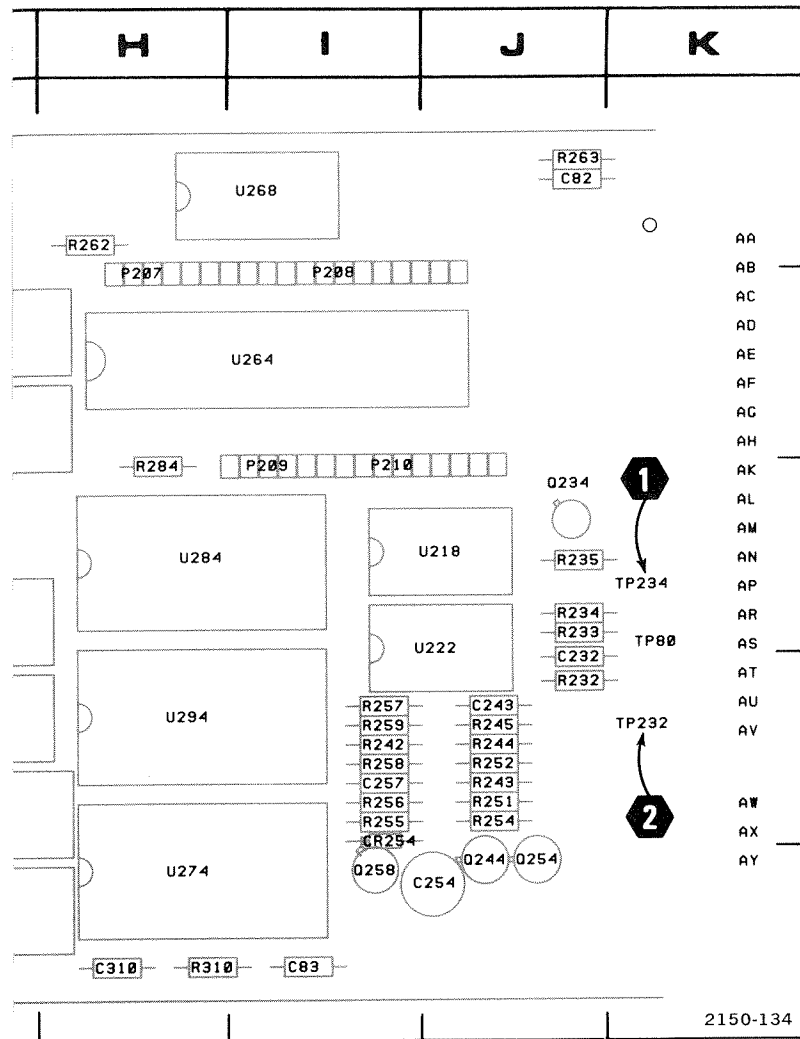

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C81	4B	R604	4B	U668	1E
C82	1J	R605	4B	U674	2B
C83	5I	R624	5C	U676	2D
C84	1E	R625	5C	U684	1C
C85	5E	R641	4B	U694	3D
C86	1B	R642	4B	VR687	2B
C87	5B	R691	3B		
C232	3J	R692	3B		
C243	4J				
C254	5J	TP80	3K		
C257	4I	TP81	1A		
C310	5H	TP82	3A		
C311	5G	TP232	4K		
C604	3B	TP234	3K		
C605	4B	TP640	5B		
C624	5C				
C625	5C	U216	3G		
C641	5B	U217	4G		
C642	4B	U218	3J		
C691	3B	U222	3J		
CR254	4I	U264	2I		
CR691	3B	U268	1I		
L81	1B	U274	5H		
P207	1H	U284	3H		
P208	1I	U294	4H		
P209	3I	U304	2G		
P210	3I	U308	4G		
		U310	5G		
		U314	1F		
		U316	2F		
		U318	4F		
		U320	5F		
		U334	3F		
		U336	2F		
		U338	4F		
		U340	3F		
		U354	2G		
R232	4J	U604	4C		
R233	3J	U614	3C		
R234	3J	U624	4D		
R235	3J	U632	3C		
R242	4I	U634	2E		
R243	4J	U636	3E		
R245	4J	U638	4E		
R251	4J	U640	4C		
R252	4J	U641	3D		
R254	4J	U642	2E		
R255	4I	U644	3E		
R256	4I	U646	4E		
R257	4I	U648	4D		
R258	4I	U652	5E		
R259	4I	U654	4E		
R262	1H	U656	3E		
R263	1J	U658	2E		
R284	3H	U662	4E		
R310	5H	U664	3E		
R311	5G	U666	2E		

locations.


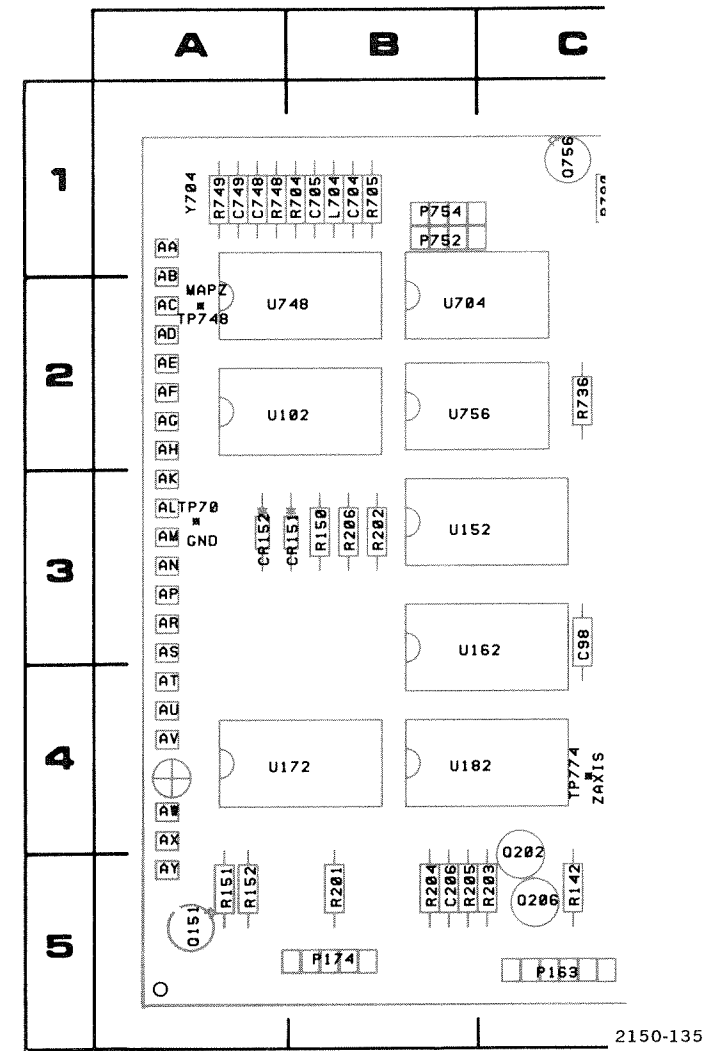


Fig. 8-7. Partial A4-Acquisition circuit board. Component locations as viewed from component side of the board.

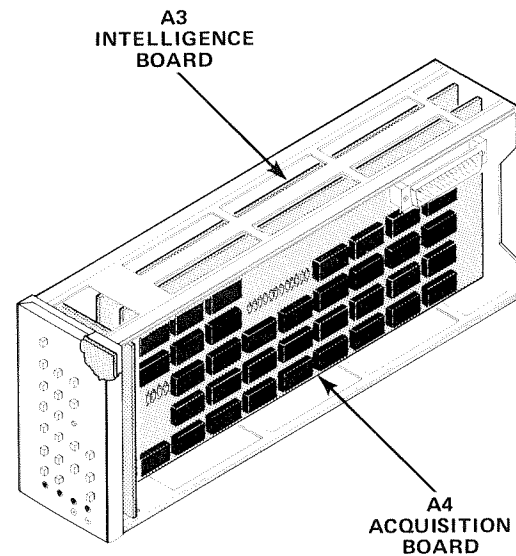


CKT NO	GRID COORD	CKT NO	GRID COORD
C206	5B	R203	5C
Q202	5C	R204	5B
Q206	5C	R205	5B
		R206	3B
R201	5B	U102	2B
R202	3B	U152	3B


VOLTAGE AND WAVEFORM CONDITIONS

Voltages and waveforms shown are typical, but may vary between instruments.

TEST SETUP: The 7D01 is connected to the 7000-series mainframe Right-Vertical and A-Horizontal compartments through two 067-0616-00 Flexible Plug-in Extenders. The DF1 is connected to the 7D01 through a 067-0805-00 Cable Extender. The DF1 is set for a STATE TABLE BINARY, 7D01 ONLY display.

The test oscilloscope is dc coupled and internally triggered.

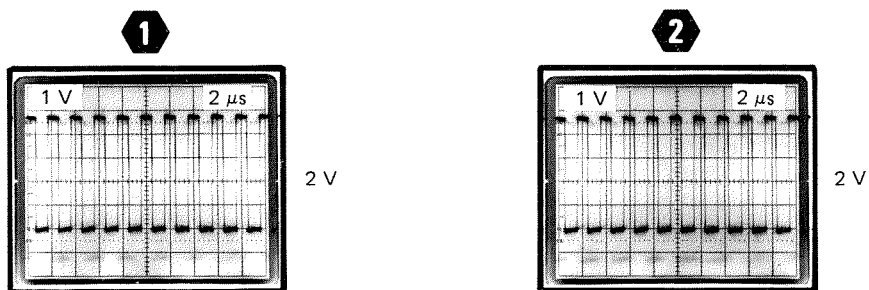

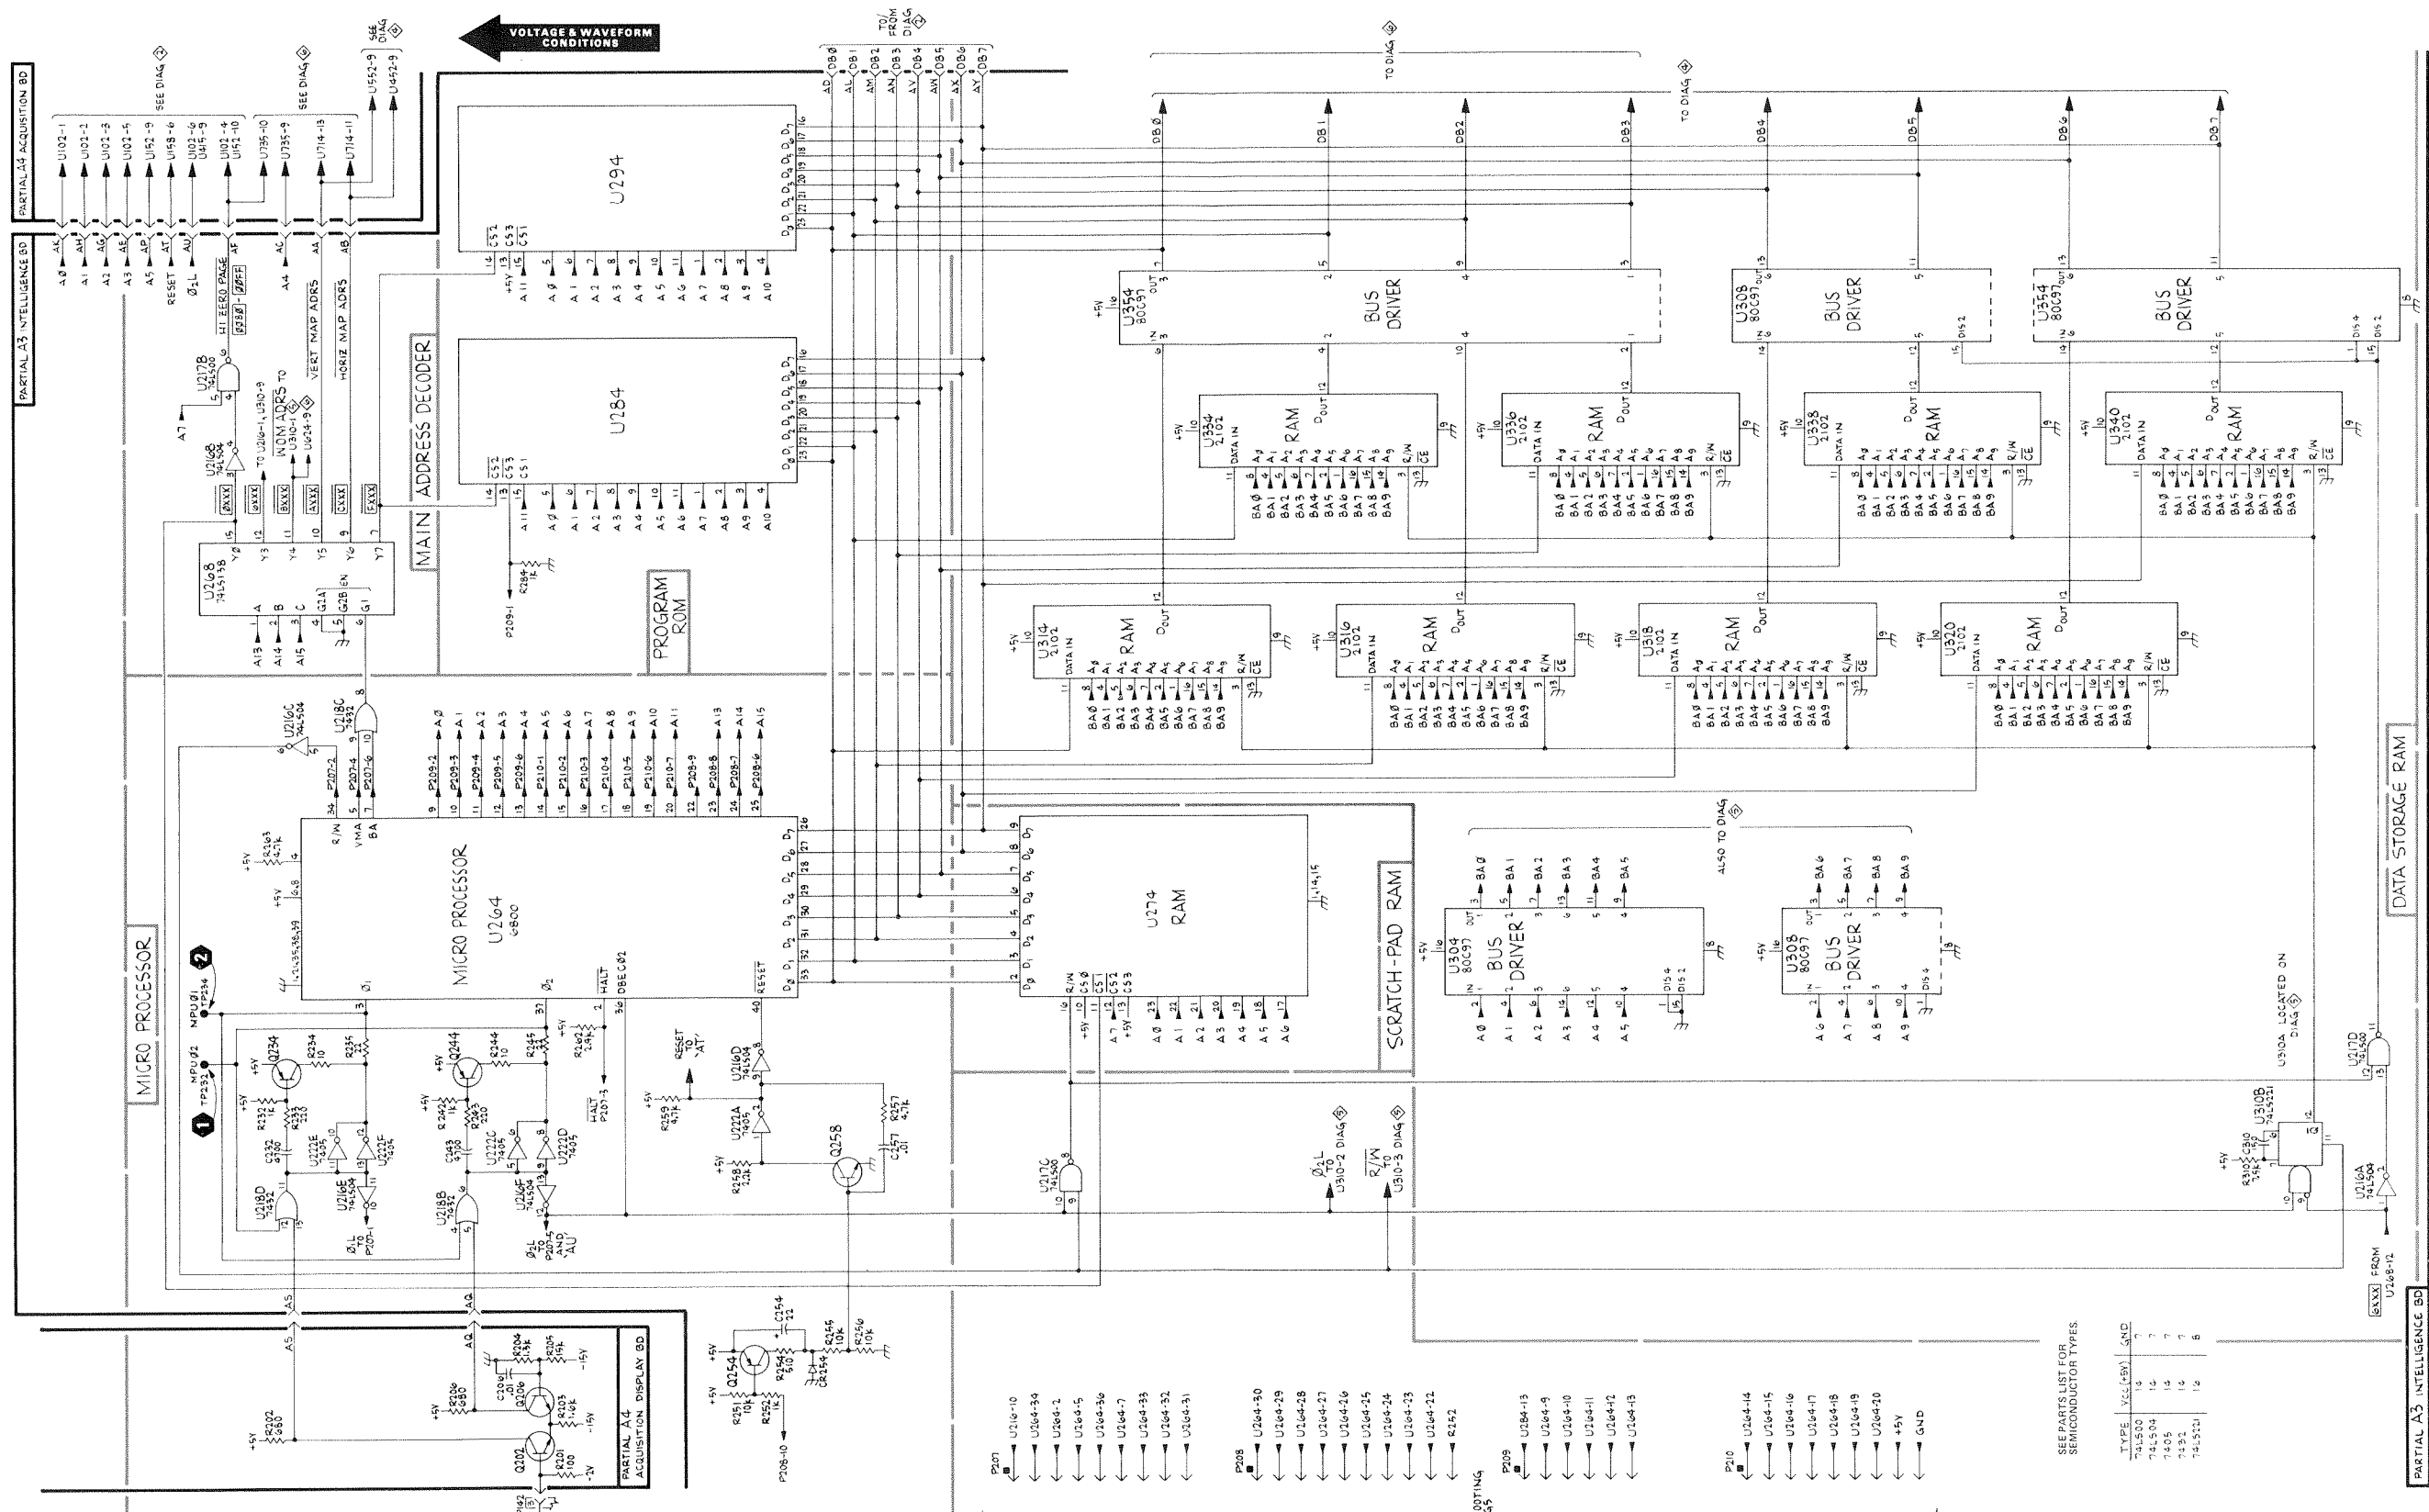

2150-20
REV. A, MAR. 1977

- TRUBLESHOOTING PLUGS
- P207
 - U216-10
 - U264-34
 - U264-39
 - U264-41
 - U264-45
 - U264-56
 - U264-7
 - U264-93
 - U264-92
 - U264-91
 - P208
 - U264-30
 - U264-29
 - U264-28
 - U264-27
 - U264-26
 - U264-25
 - U264-24
 - U264-23
 - U264-22
 - R252
 - P209
 - U284-13
 - U284-9
 - U284-10
 - U284-11
 - U284-12
 - U284-13
 - P210
 - U264-14
 - U264-15
 - U264-16
 - U264-17
 - U264-18
 - U264-19
 - U264-20
 - +5V
 - GND

SEE PARTS LIST FOR SEMICONDUCTOR TYPES

TYPE	VAL (CV)	AND
74LS00	14	7
74LS04	14	7
7405	14	7
7492	14	7
74LS121	12	5

PARTIAL A3 INTELLIGENCE BD


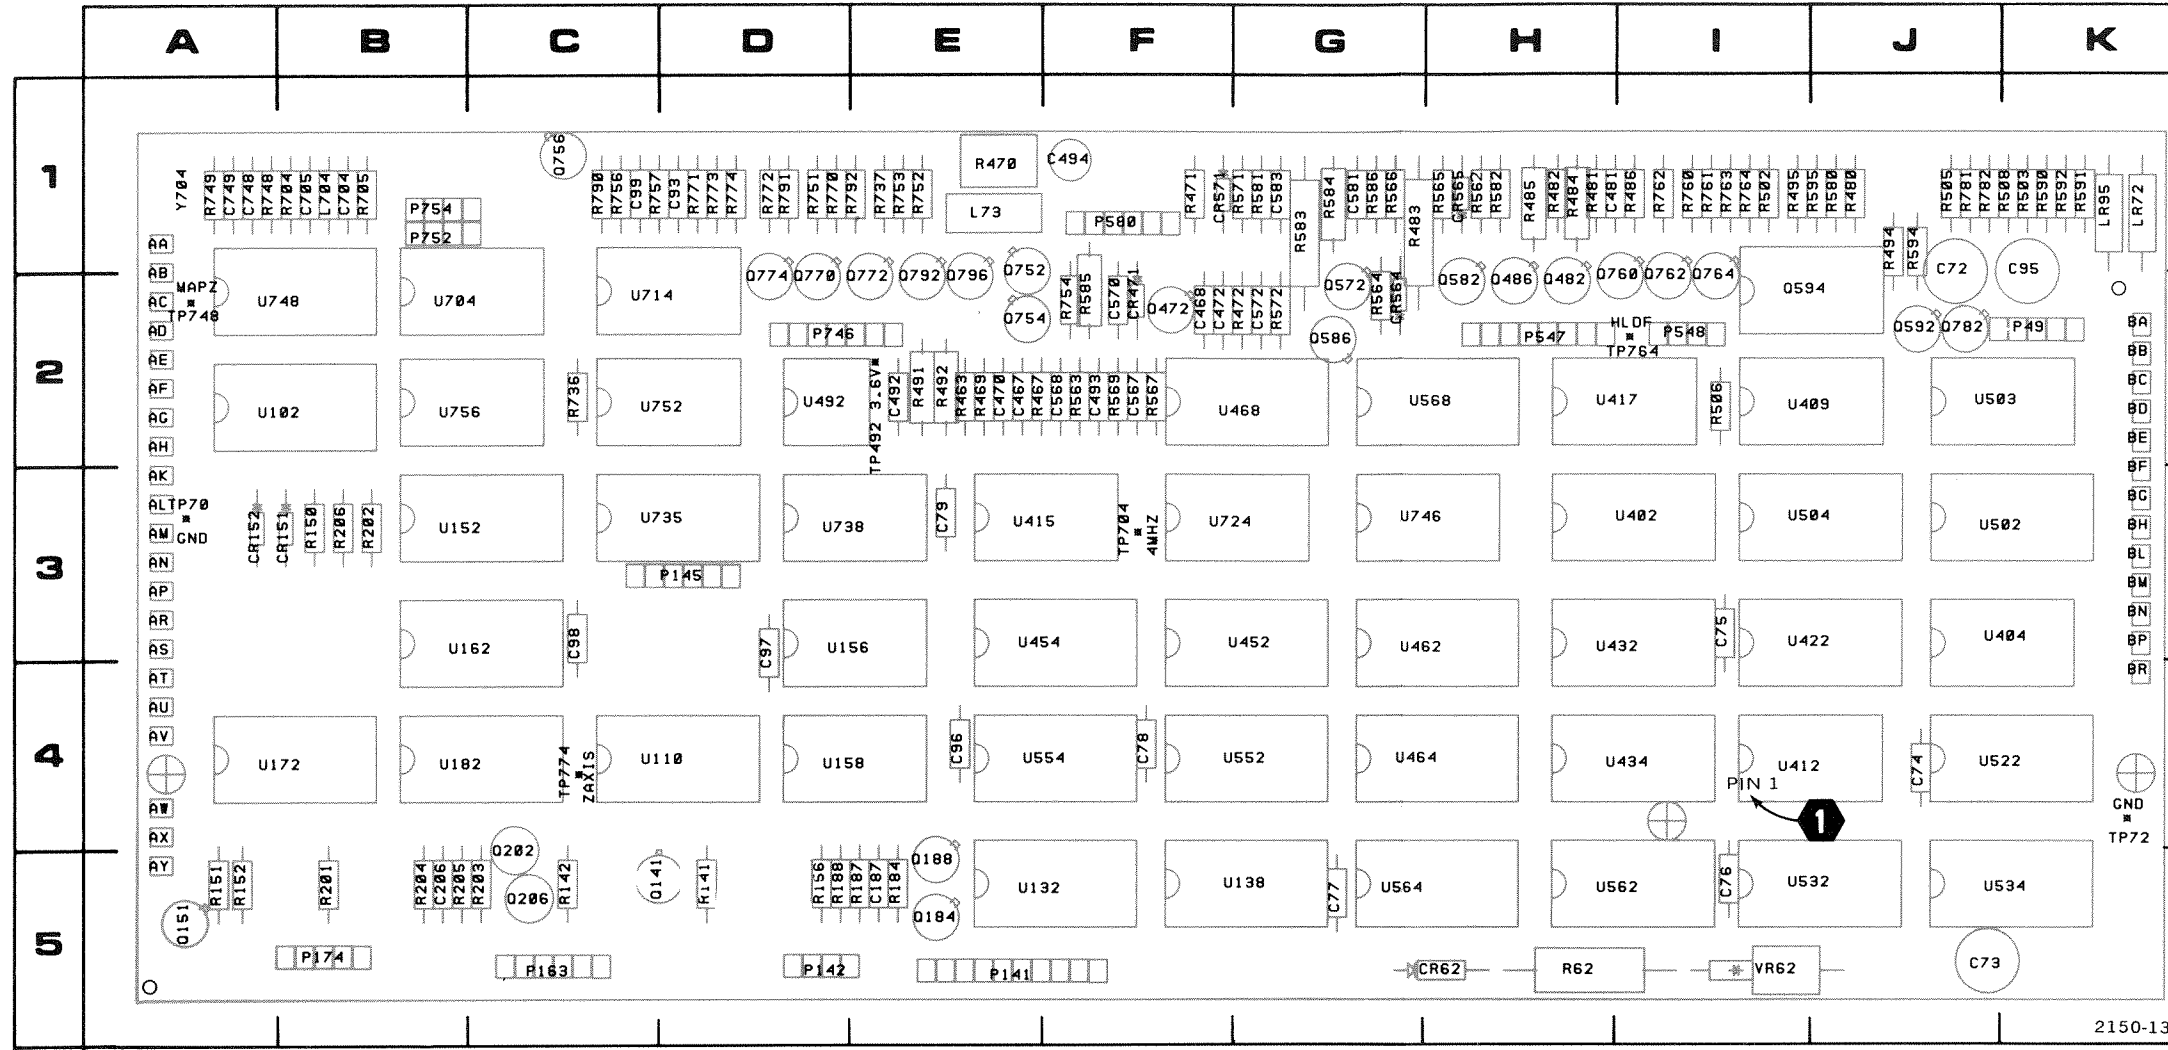



Figure 8-8. A4—Acquisition circuit board component locations.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C72	1J	Q141	5C	R503	1K	U110	4C
C73	5J	Q151	5A	R505	1J	U132	5E
C74	4J	Q184	5E	R506	2I	U138	5G
C75	3I	Q188	5E	R508	1K	U152	3B
C76	5I	Q202	5C	R562	1H	U156	3D
C77	5G	Q206	5C	R563	2F	U158	4D
C78	4F	Q472	2F	R564	2G	U162	3B
C79	3E	Q482	2H	R565	1H	U172	4A
C93	1D	Q486	2H	R566	1G	U182	4B
C95	1K	Q572	2G	R567	2F	U402	3I
C96	4E	Q582	2H	R569	2F	U404	3K
C97	3D	Q586	2G	R571	1G	U409	2I
C98	3C	Q592	2I	R572	2G	U412	4I
C99	1C	Q594	2I	R580	1J	U415	3E
C187	5E	Q752	1E	R581	1G	U417	2I
C206	5B	Q754	2E	R582	1H	U422	3I
C467	2E	Q756	1C	R583	1G	U432	3I
C468	2F	Q760	2I	R584	1G	U434	4I
C470	2E	Q762	2I	R585	2F	U452	3E
C472	2F	Q764	2I	R586	1G	U454	3E
C481	1H	Q770	2D	R590	1K	U462	3G
C492	2E	Q772	2E	R591	1K	U464	4H
C493	2F	Q774	2D	R592	1K	U468	2F
C494	1F	Q782	2I	R594	1J	U492	2D
C567	2F	Q792	2E	R595	1J	U502	3K
C568	2F	Q796	2E	R704	1B	U503	2I
C570	2F			R705	1B	U504	3I
C572	2G	R62	5H	R736	2C	U522	4K
C581	1G	R141	5D	R737	1E	U532	5I
C583	1G	R142	5C	R748	1A	U534	5J
C704	1B	R150	3B	R749	1A	U552	4G
C705	1B	R151	5A	R751	1D	U554	4E
C748	1A	R152	5A	R752	1E	U562	5I
C749	1A	R156	5D	R753	1E	U564	5G
		R184	5E	R754	2F	U568	2H
CR62	5H	R187	5E	R756	1C	U704	2B
CR151	3B	R188	5D	R757	1C	U714	2C
CR152	3A	R201	5B	R760	1I	U724	3E
CR471	2F	R202	3B	R761	1I	U735	3D
CR564	2G	R203	5C	R762	1I	U738	3D
CR565	1H	R204	5B	R763	1I	U746	3G
CR571	1F	R205	5B	R764	1I	U748	2B
		R206	3B	R770	1D	U752	2C
L73	1E	R463	2E	R771	1D	U756	2B
L704	1B	R467	2E	R772	1D		
		R469	2E	R773	1D	VR62	5I
LR72	1K	R470	1E	R774	1D		
LR95	1K	R471	1F	R781	1J	Y704	1A
		R472	2F	R790	1C		

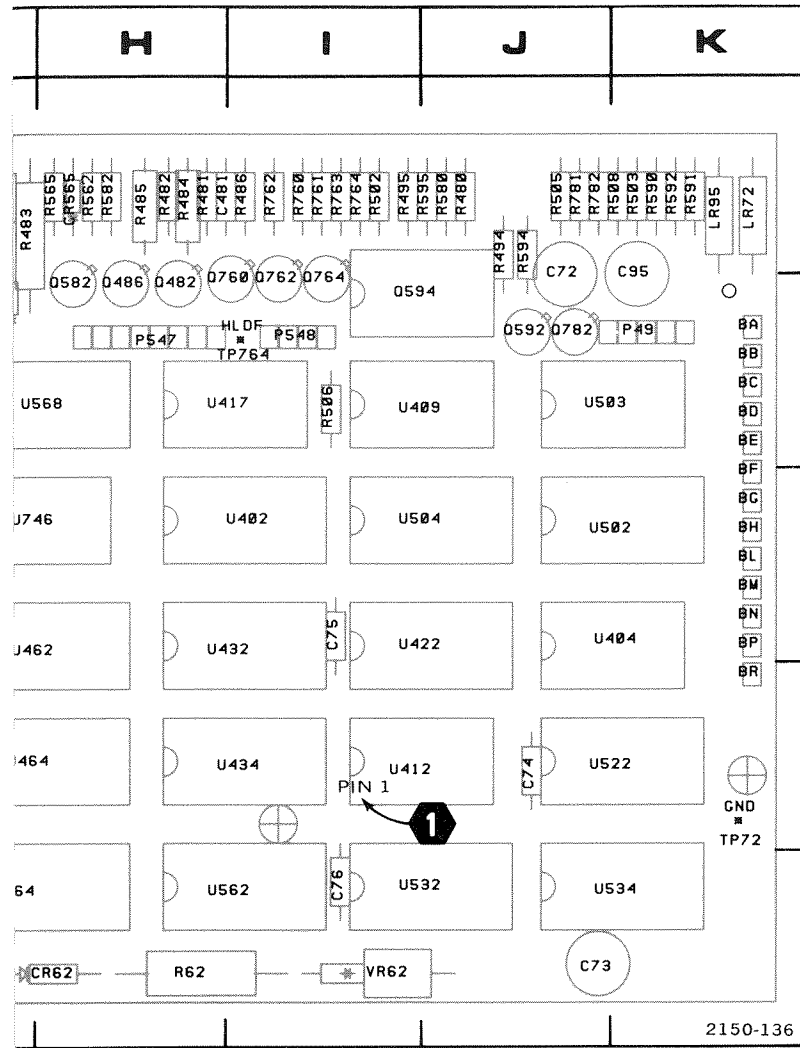

nt locations.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C72	1J	Q141	5C	R503	1K	U110	4C
C73	5J	Q151	5A	R505	1J	U132	5E
C74	4J	Q184	5E	R506	2I	U138	5G
C75	3I	Q188	5E	R508	1K	U152	3B
C76	5I	Q202	5C	R562	1H	U156	3D
C77	5G	Q206	5C	R563	2F	U158	4D
C78	4F	Q472	2F	R564	2G	U162	3B
C79	3E	Q482	2H	R565	1H	U172	4A
C93	1D	Q486	2H	R566	1G	U182	4B
C95	1K	Q572	2G	R567	2F	U402	3I
C96	4E	Q582	2H	R569	2F	U404	3K
C97	3D	Q586	2G	R571	1G	U409	2I
C98	3C	Q592	2I	R572	2G	U412	4I
C99	1C	Q594	2I	R580	1J	U415	3E
C187	5E	Q752	1E	R581	1G	U417	2I
C206	5B	Q754	2E	R582	1H	U422	3I
C467	2E	Q756	1C	R583	1G	U432	3I
C468	2F	Q760	2I	R584	1G	U434	4I
C470	2E	Q762	2I	R585	2F	U452	3E
C472	2F	Q764	2I	R586	1G	U454	3E
C481	1H	Q770	2D	R590	1K	U462	3G
C492	2E	Q772	2E	R591	1K	U464	4H
C493	2F	Q774	2D	R592	1K	U468	2F
C494	1F	Q782	2I	R594	1J	U492	2D
C567	2F	Q792	2E	R595	1J	U502	3K
C568	2F	Q796	2E	R704	1B	U503	2I
C570	2F			R705	1B	U504	3I
C572	2G	R62	5H	R736	2C	U522	4K
C581	1G	R141	5D	R737	1E	U532	5I
C583	1G	R142	5C	R748	1A	U534	5J
C704	1B	R150	3B	R749	1A	U552	4G
C705	1B	R151	5A	R751	1D	U554	4E
C748	1A	R152	5A	R752	1E	U562	5I
C749	1A	R156	5D	R753	1E	U564	5G
		R184	5E	R754	2F	U568	2H
CR62	5H	R187	5E	R756	1C	U704	2B
CR151	3B	R188	5D	R757	1C	U714	2C
CR152	3A	R201	5B	R760	1I	U724	3E
CR471	2F	R202	3B	R761	1I	U735	3D
CR564	2G	R203	5C	R762	1I	U738	3D
CR565	1H	R204	5B	R763	1I	U746	3G
CR571	1F	R205	5B	R764	1I	U748	2B
		R206	3B	R770	1D	U752	2C
		R463	2E	R771	1D	U756	2B
L73	1E	R467	2E	R772	1D		
L704	1B	R469	2E	R773	1D	VR62	5I
		R470	1E	R774	1D		
LR72	1K	R471	1F	R781	1J	Y704	1A
LR95	1K	R472	2F	R790	1C		
		R480	1J	R791	1D		
P49	2K	R481	1H	R792	1E		
P141	5E	R482	1H				
P142	5D	R483	1G	TP70	3A		
P145	3D	R484	1H	TP72	4K		
P163	5C	R485	1H	TP492	2E		
P174	5B	R486	1I	TP704	3E		
P547	2H	R491	2E	TP748	2A		
P548	2I	R492	2E	TP764	2I		
P580	1F	R494	1J	TP774	4C		
P746	2D	R495	1I				
P752	1B	R502	1I	U102	2B		
P754	1B						

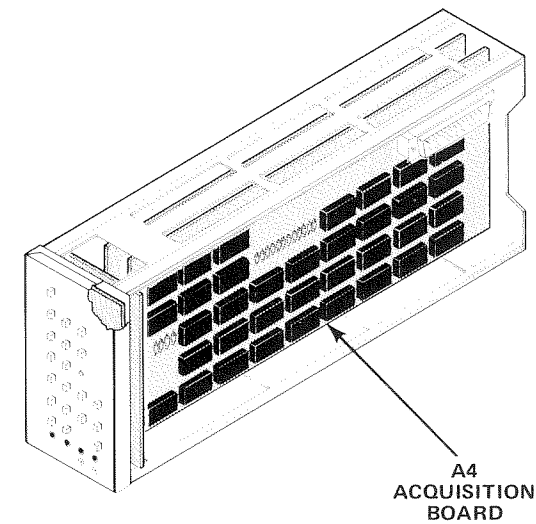



VOLTAGE AND WAVEFORM CONDITIONS

Voltages and waveforms shown are typical, but may vary between instruments.

TEST SETUP: The 7D01 is connected to the 7000-series mainframe Right-Vertical and A-Horizontal compartments through two 067-0616-00 Flexible Plug-in Extenders. The DF1 is connected to the 7D01 through a 067-0805-00 Cable Extender. The DF1 is set for a STATE TABLE BINARY, 7D01 ONLY display.

The test oscilloscope is dc coupled and internally triggered.

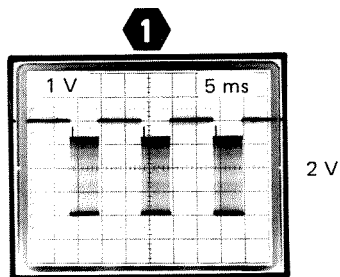

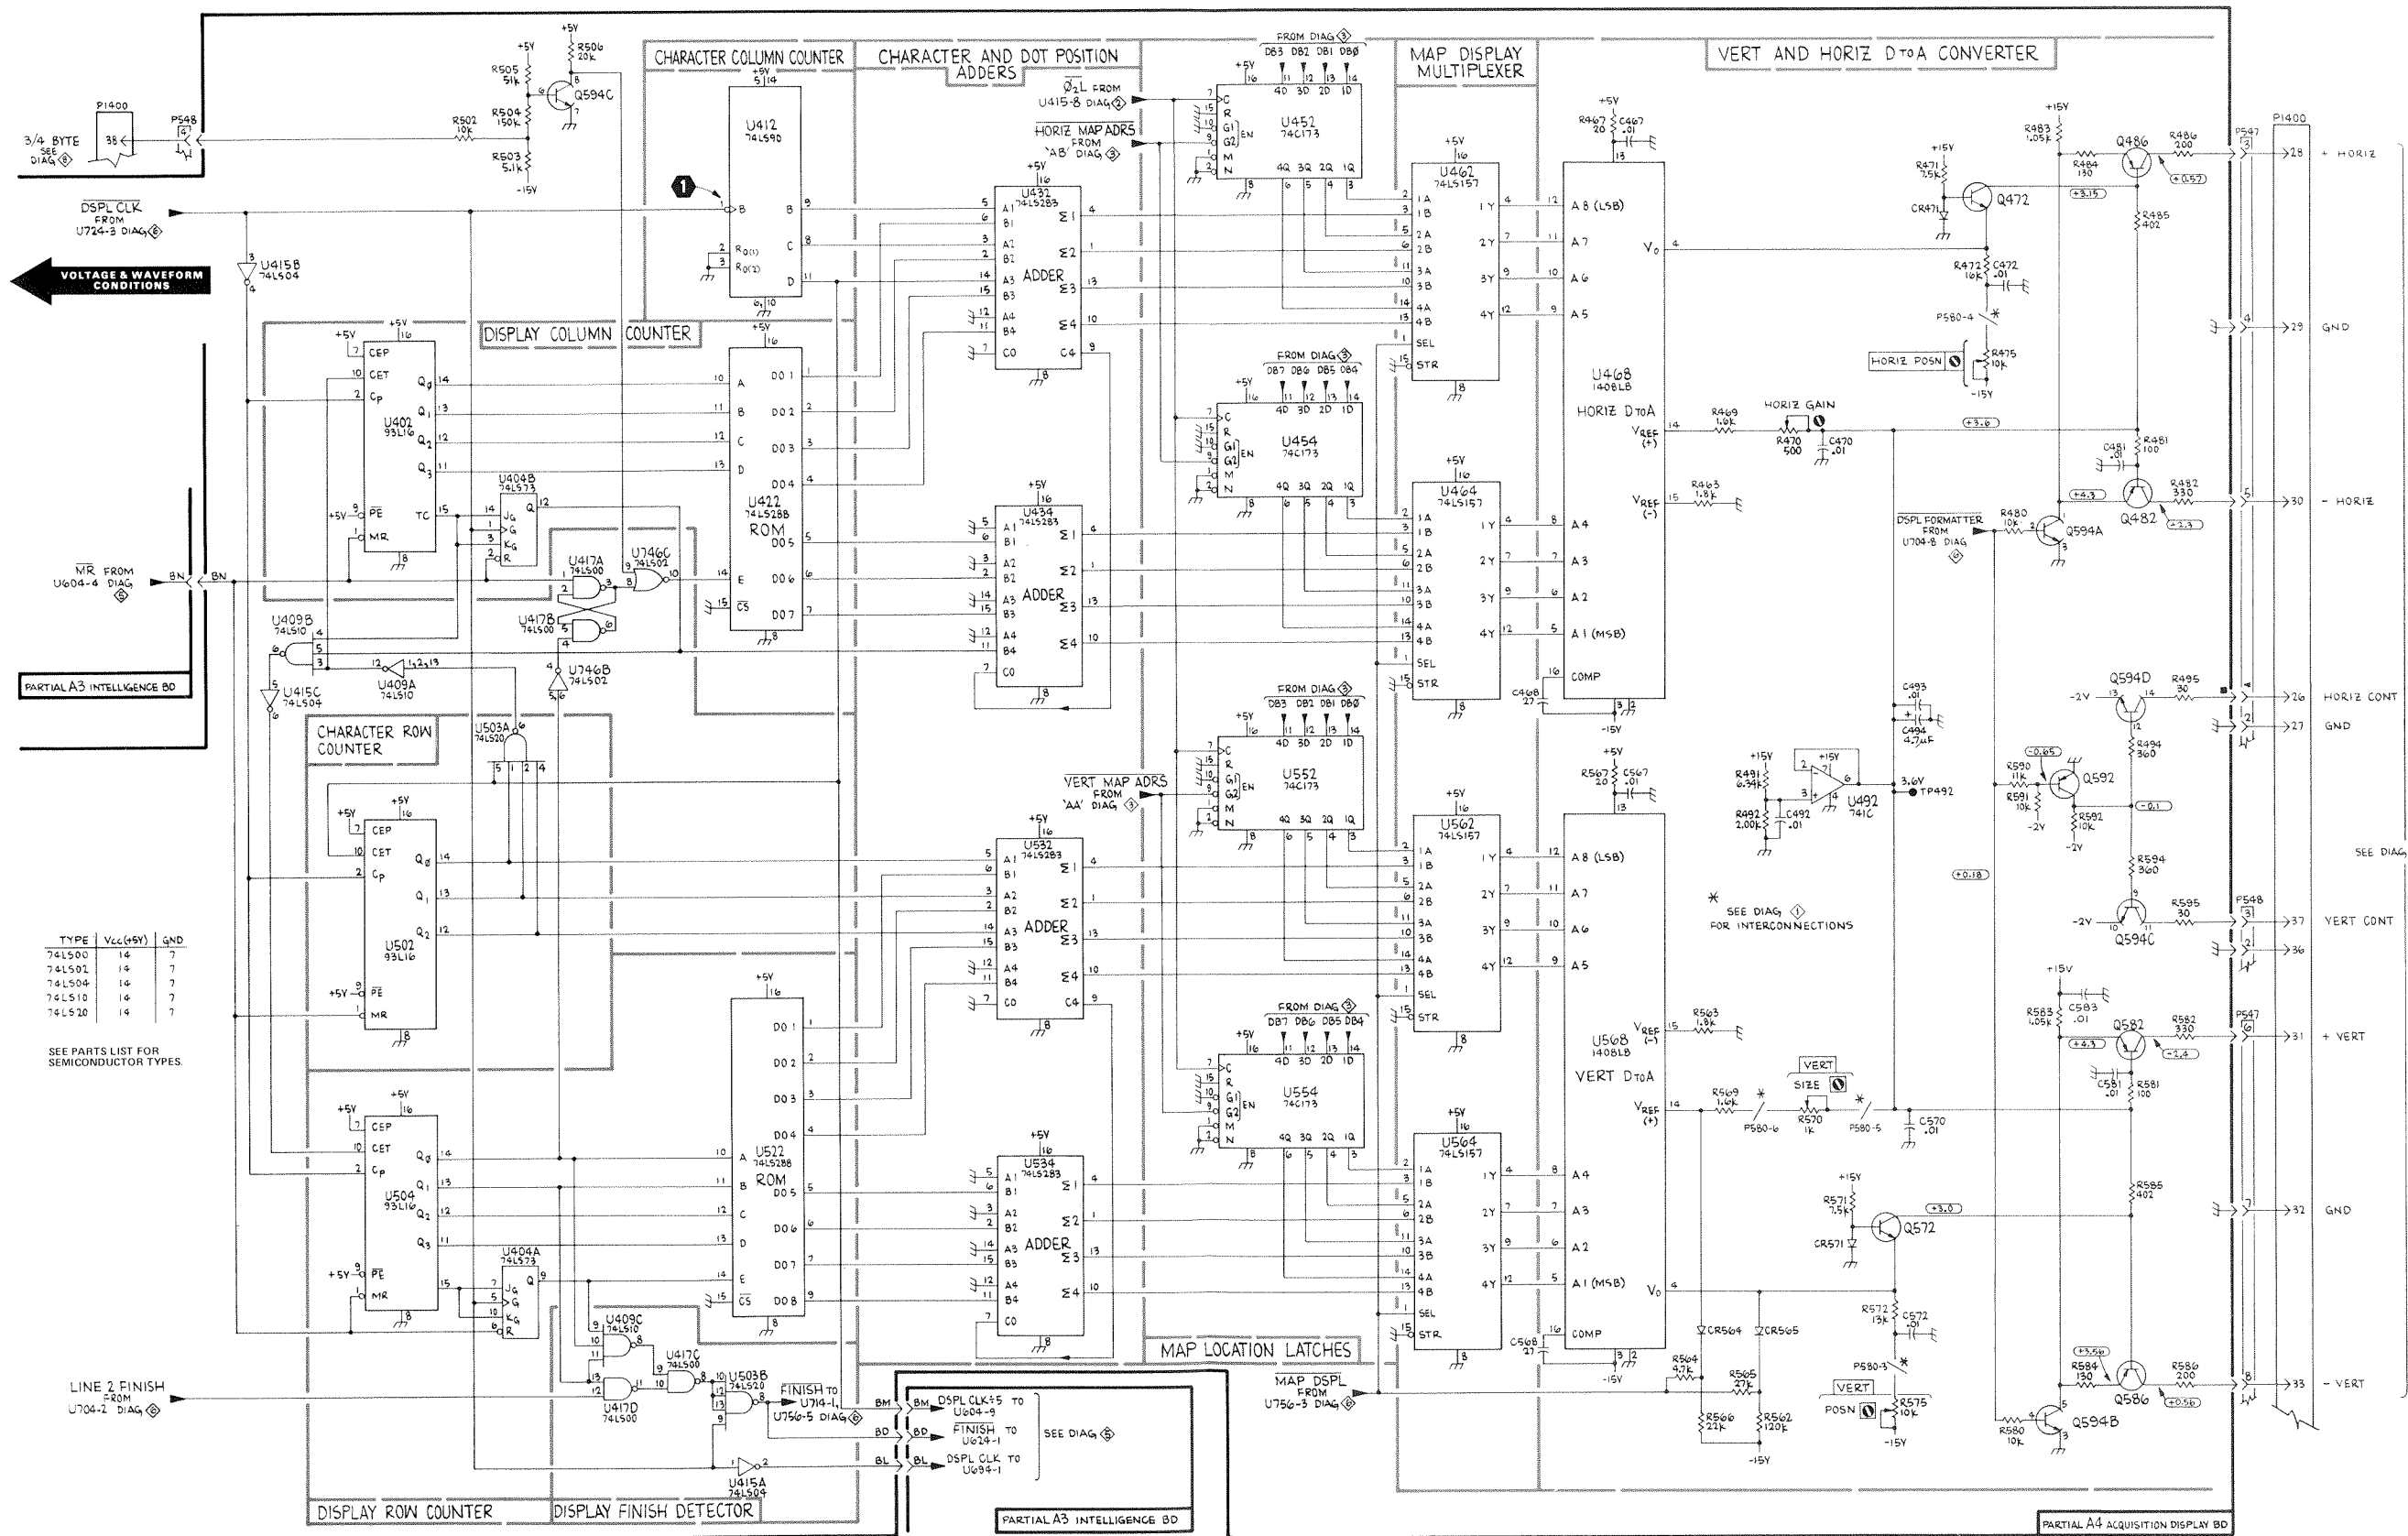

TYPE	V _{CC} (+5V)	GND
74LS00	14	7
74LS01	14	7
74LS04	14	7
74LS10	14	7
74LS20	14	7

SEE PARTS LIST FOR SEMICONDUCTOR TYPES



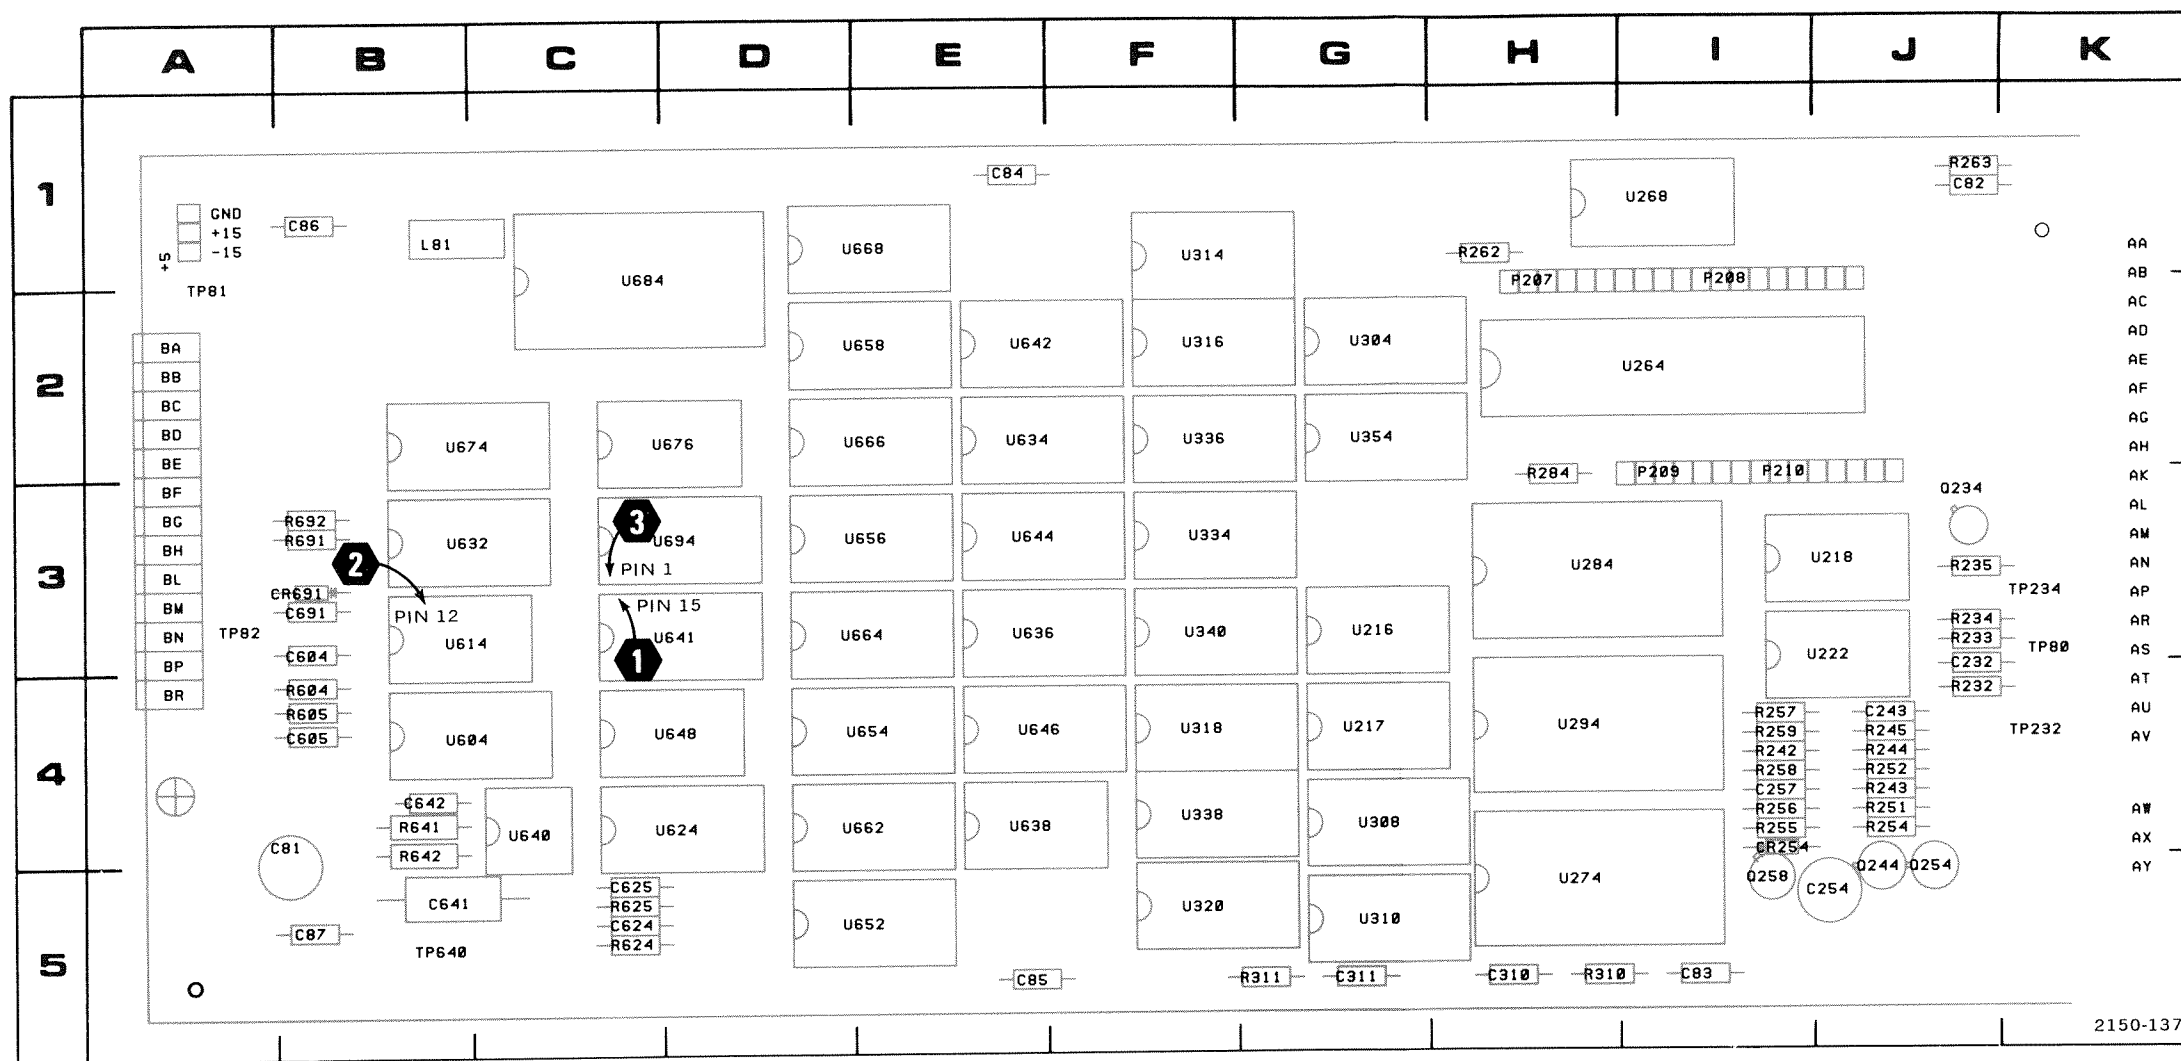


Figure 8-9. A3-Intelligence circuit board component locations.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C81	4B	R604	4B	U668	1E
C82	1J	R605	4B	U674	2B
C83	5I	R624	5C	U676	2D
C84	1E	R625	5C	U684	1C
C85	5E	R641	4B	U694	3D
C86	1B	R642	4B		
C87	5B	R691	3B	VR687	
C232	3J	R692	3B		
C243	4J				
C254	5J	TP80	3K		
C257	4I	TP81	1A		
C310	5H	TP82	3A		
C311	5G	TP232	4K		
C604	3B	TP234	3K		
C605	4B	TP640	5B		
C624	5C				
C625	5C	U216	3G		
C641	5B	U217	4G		
C642	4B	U218	3J		
C691	3B	U222	3J		
		U264	2I		
CR254	4I	U268	1I		
CR691	3B	U274	5H		
		U284	3H		
L81	1B	U294	4H		
		U304	2G		
P207	1H	U308	4G		
P208	1I	U310	5G		
P209	3I	U314	1F		
P210	3I	U316	2F		
		U318	4F		
Q234	3J	U320	5F		
Q244	5J	U334	3F		
Q254	5J	U336	2F		
Q258	5I	U338	4F		
		U340	3F		
R232	4J	U354	2G		
R233	3J	U604	4C		
R234	3J	U614	3C		
R235	3J	U624	4D		
R242	4I	U632	3C		
R243	4J	U634	2E		
R244	4J	U636	3E		
R245	4J	U638	4E		
R251	4J	U640	4C		
R252	4J	U641	3D		
R254	4J	U642	2E		
R255	4I	U644	3E		
R256	4I	U646	4E		
R257	4I	U648	4D		
R258	4I	U652	5E		
R259	4I	U654	4E		
R262	1H	U656	3E		
R263	1J	U658	2E		
R284	3H	U662	4E		
R310	5H	U664	3E		
R311	5G	U666	2E		

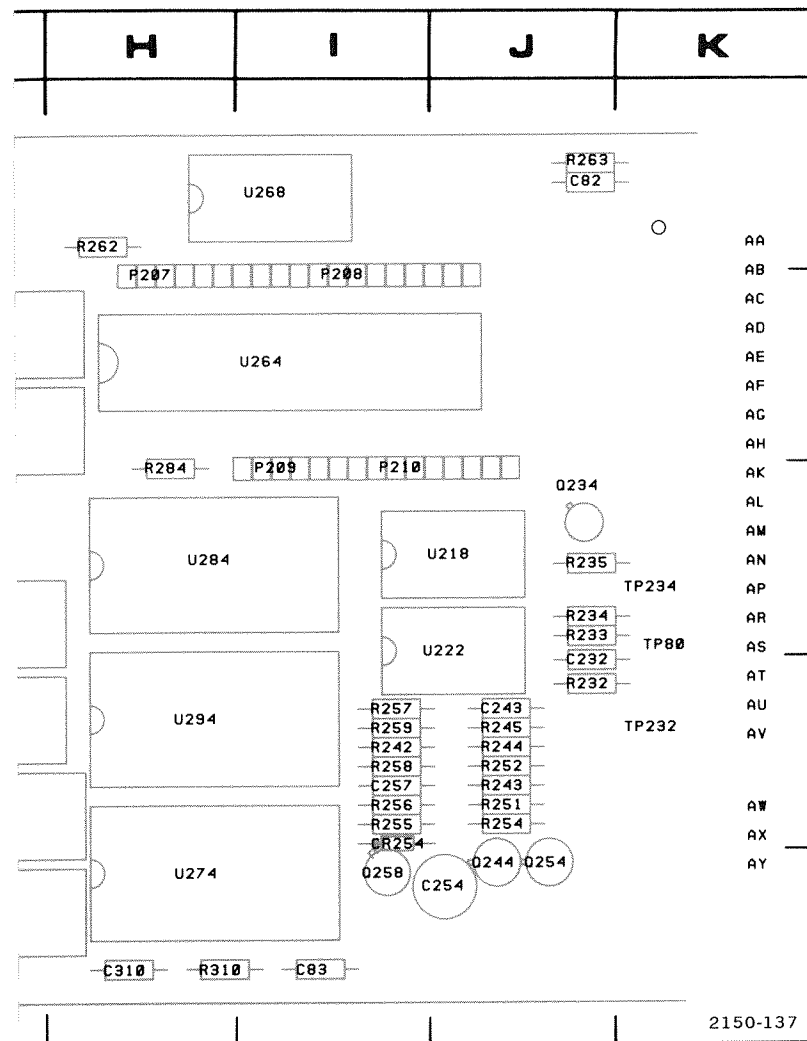

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C81	4B	R604	4B	U668	1E
C82	1J	R605	4B	U674	2B
C83	5I	R624	5C	U676	2D
C84	1E	R625	5C	U684	1C
C85	5E	R641	4B	U694	3D
C86	1B	R642	4B		
C87	5B	R691	3B	VR687	
C232	3J	R692	3B		
C243	4J				
C254	5J	TP80	3K		
C257	4I	TP81	1A		
C310	5H	TP82	3A		
C311	5G	TP232	4K		
C604	3B	TP234	3K		
C605	4B	TP640	5B		
C624	5C				
C625	5C	U216	3G		
C641	5B	U217	4G		
C642	4B	U218	3J		
C691	3B	U222	3J		
		U264	2I		
CR254	4I	U268	1I		
CR691	3B	U274	5H		
		U284	3H		
L81	1B	U294	4H		
		U304	2G		
P207	1H	U308	4G		
P208	1I	U310	5G		
P209	3I	U314	1F		
P210	3I	U316	2F		
		U318	4F		
Q234	3J	U320	5F		
Q244	5J	U334	3F		
Q254	5J	U336	2F		
Q258	5I	U338	4F		
		U340	3F		
R232	4J	U354	2G		
R233	3J	U604	4C		
R234	3J	U614	3C		
R235	3J	U624	4D		
R242	4I	U632	3C		
R243	4J	U634	2E		
R244	4J	U636	3E		
R245	4J	U638	4E		
R251	4J	U640	4C		
R252	4J	U641	3D		
R254	4J	U642	2E		
R255	4I	U644	3E		
R256	4I	U646	4E		
R257	4I	U648	4D		
R258	4I	U652	5E		
R259	4I	U654	4E		
R262	1H	U656	3E		
R263	1J	U658	2E		
R284	3H	U662	4E		
R310	5H	U664	3E		
R311	5G	U666	2E		

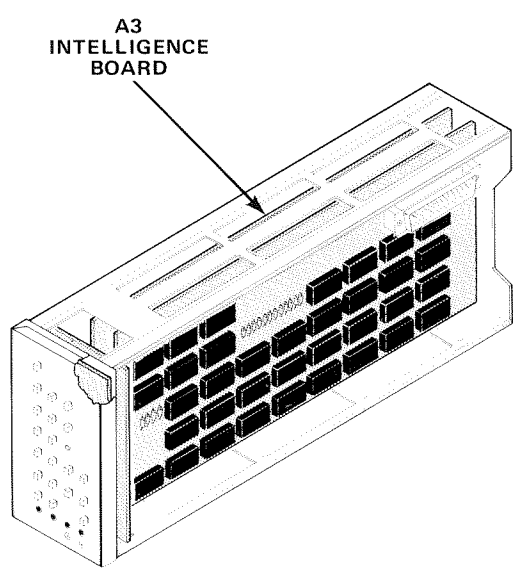


ations.


VOLTAGE AND WAVEFORM CONDITIONS

Voltages and waveforms shown are typical, but may vary between instruments.

TEST SETUP: The 7D01 is connected to the 7000-series mainframe Right-Vertical and A-Horizontal compartments through two 067-0616-00 Flexible Plug-in Extenders. The DF1 is connected to the 7D01 through a 067-0805-00 Cable Extender. The DF1 is set for a STATE TABLE BINARY, 7D01 ONLY display.

The test oscilloscope is dc coupled and internally triggered.

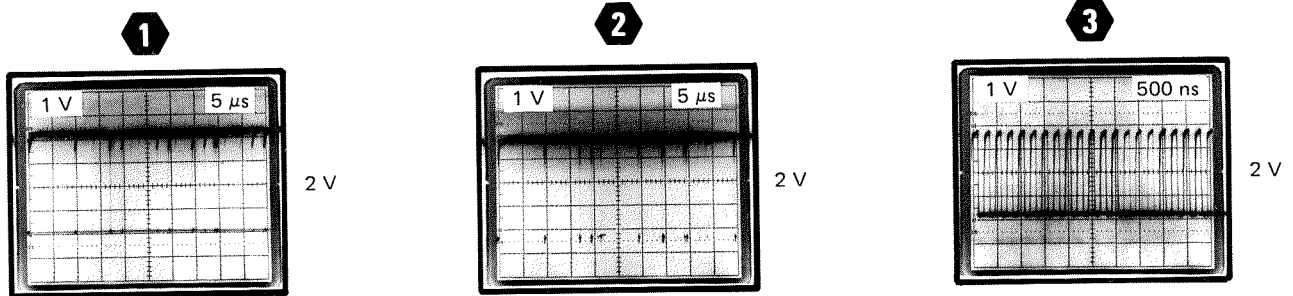

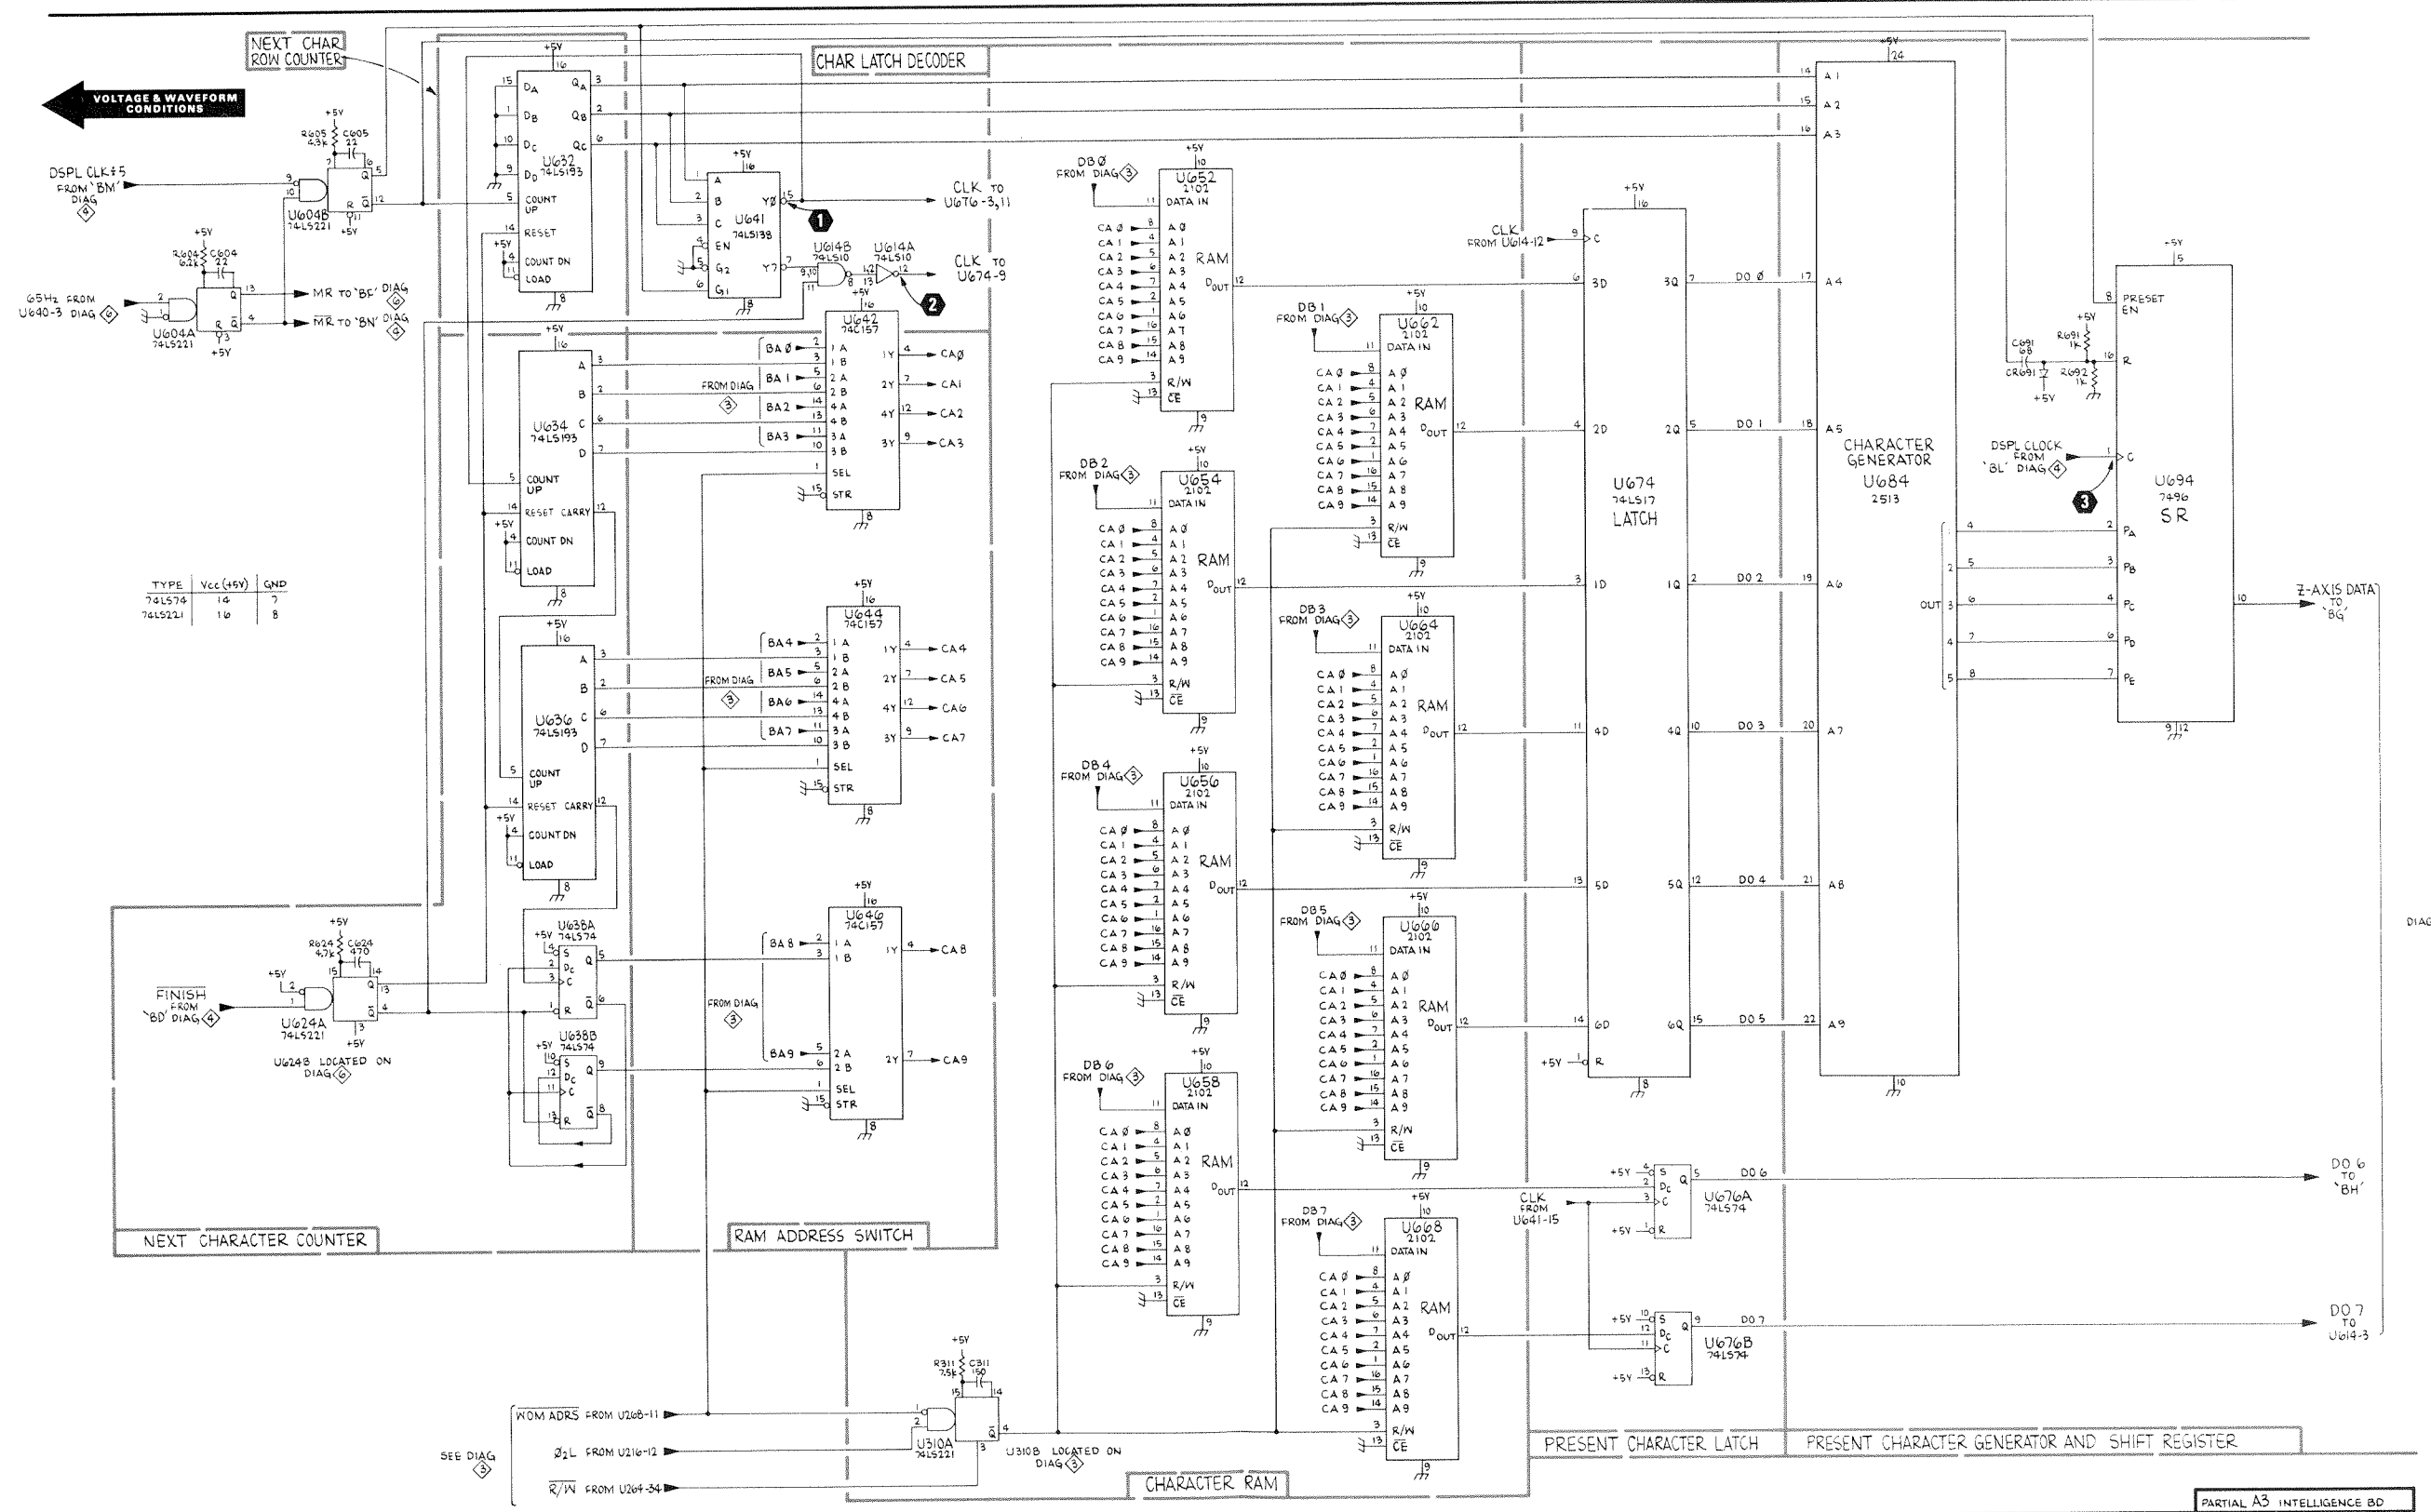


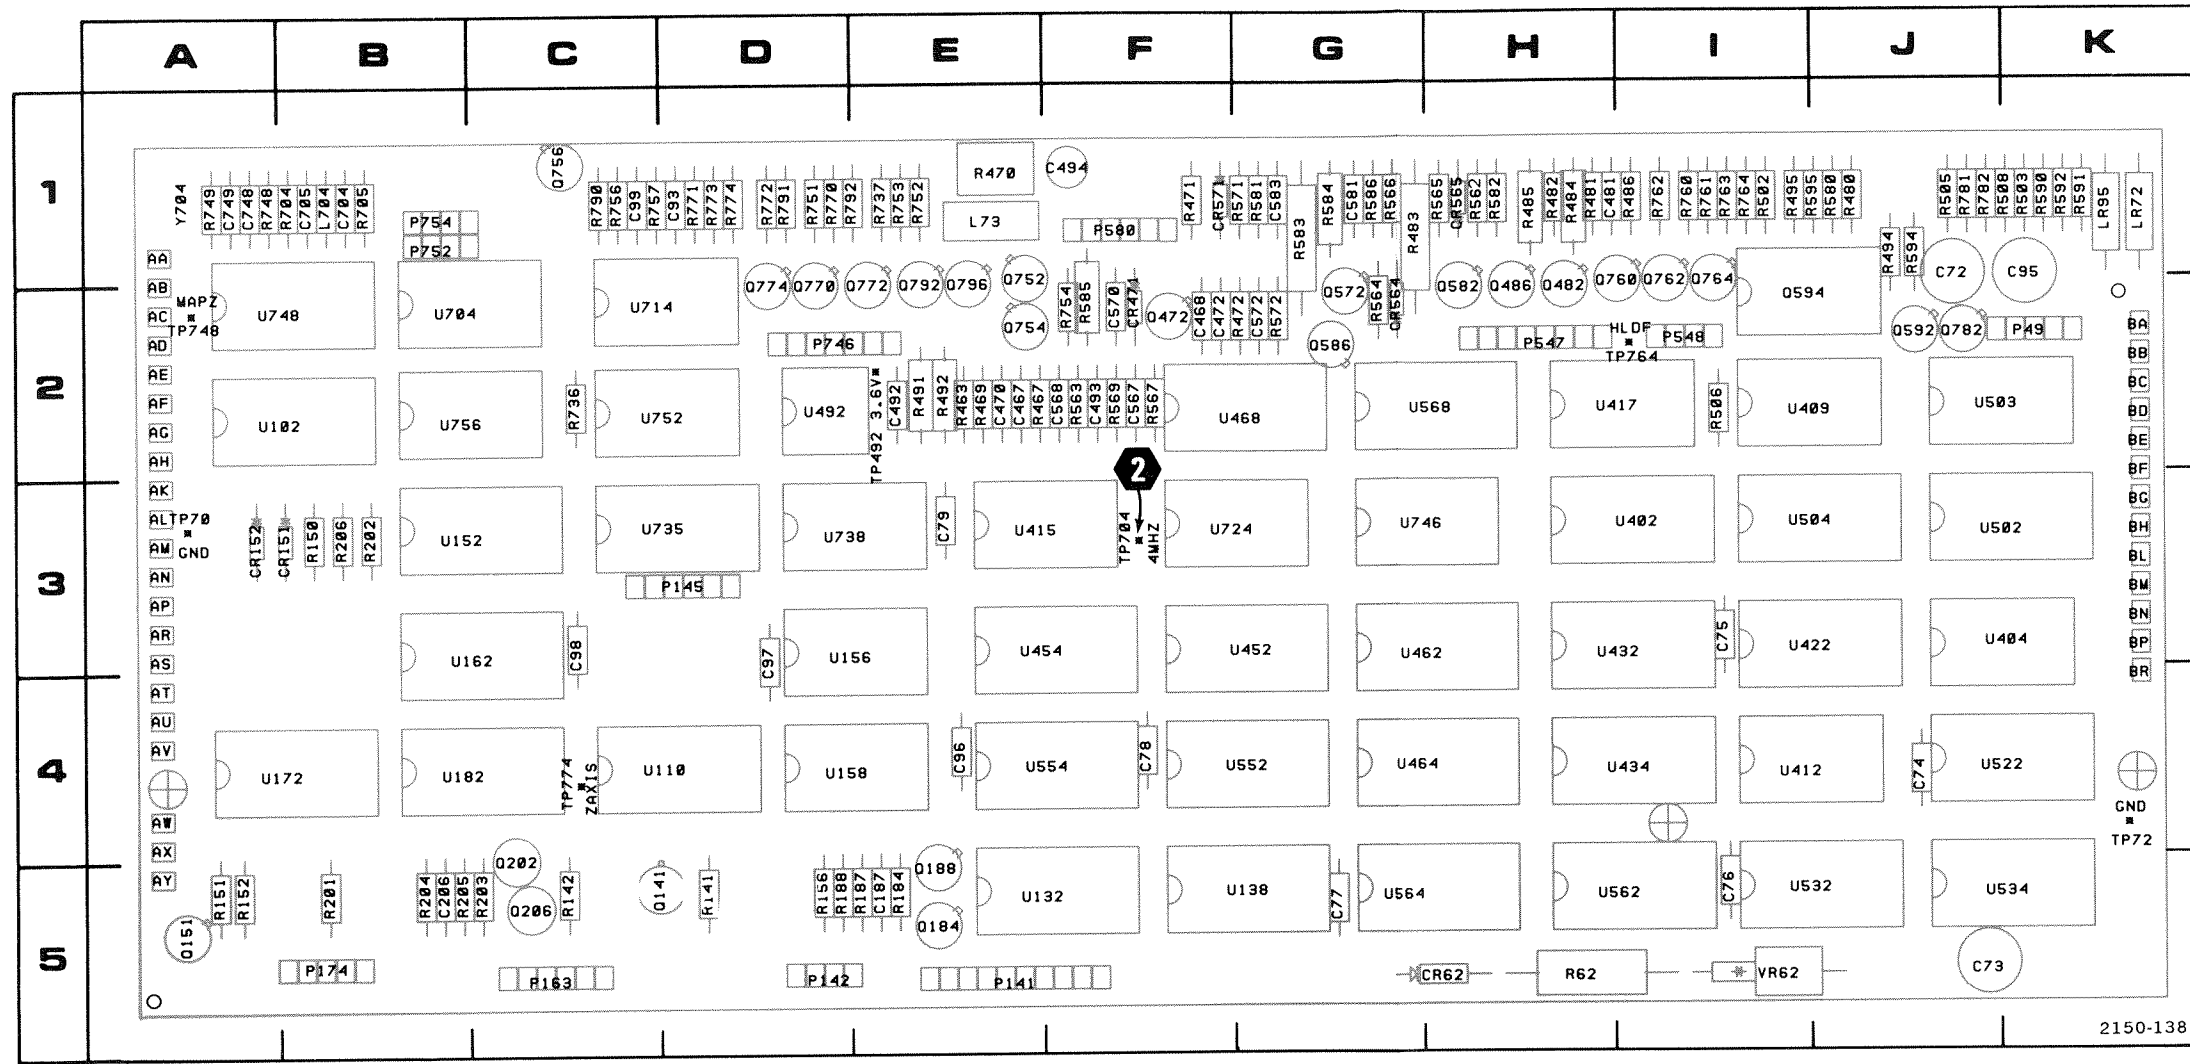


Figure 8-10. A4—Acquisition circuit board component locations.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C72	1J	Q141	5C	R503	1K	U110	4C
C73	5J	Q151	5A	R505	1J	U132	5E
C74	4J	Q184	5E	R506	2I	U138	5G
C75	3I	Q188	5E	R508	1K	U152	3B
C76	5I	Q202	5C	R562	1H	U156	3D
C77	5G	Q206	5C	R563	2F	U158	4D
C78	4F	Q472	2F	R564	2G	U162	3B
C79	3E	Q482	2H	R565	1H	U172	4A
C93	1D	Q486	2H	R566	1G	U182	4B
C95	1K	Q572	2G	R567	2F	U402	3I
C96	4E	Q582	2H	R569	2F	U404	3K
C97	3D	Q586	2G	R571	1G	U409	2I
C98	3C	Q592	2I	R572	2G	U412	4I
C99	1C	Q594	2I	R580	1J	U415	3E
C187	5E	Q752	1E	R581	1G	U417	2I
C206	5B	Q754	2E	R582	1H	U422	3I
C467	2E	Q756	1C	R583	1G	U432	3I
C468	2F	Q760	2I	R584	1G	U434	4I
C470	2E	Q762	2I	R585	2F	U452	3E
C472	2F	Q764	2I	R586	1G	U454	3E
C481	1H	Q770	2D	R590	1K	U462	3G
C492	2E	Q772	2E	R591	1K	U464	4H
C493	2F	Q774	2D	R592	1K	U468	2F
C494	1F	Q782	2I	R594	1J	U492	2D
C567	2F	Q792	2E	R595	1J	U502	3K
C568	2F	Q796	2E	R704	1B	U503	2I
C570	2F			R705	1B	U504	3I
C572	2G	R62	5H	R736	2C	U522	4K
C581	1G	R141	5D	R737	1E	U532	5I
C583	1G	R142	5C	R748	1A	U534	5J
C704	1B	R150	3B	R749	1A	U552	4G
C705	1B	R151	5A	R751	1D	U554	4E
C748	1A	R152	5A	R752	1E	U562	5I
C749	1A	R156	5D	R753	1E	U564	5G
		R184	5E	R754	2F	U568	2H
CR62	5H	R187	5E	R756	1C	U704	2B
CR151	3B	R188	5D	R757	1C	U714	2C
CR152	3A	R201	5B	R760	1I	U724	3E
CR471	2F	R202	3B	R761	1I	U735	3D
CR564	2G	R203	5C	R762	1I	U738	3D
CR565	1H	R204	5B	R763	1I	U746	3G
CR571	1F	R205	5B	R764	1I	U748	2B
		R206	3B	R770	1D	U752	2C
L73	1E	R463	2E	R771	1D	U756	2B
L704	1B	R467	2E	R772	1D		
		R469	2E	R773	1D	VR62	5I
LR72	1K	R470	1E	R774	1D		
LR95	1K	R471	1F	R781	1J	Y704	1A
		R472	2F	R790	1C		
P49	2K	R480	1J	R791	1D		
P141	5E	R481	1H	R792	1E		
P142	5D	R482	1H				
P145	3D	R483	1G	TP70	3A		
P163	5C	R484	1H	TP72	4K		
P174	5B	R485	1H	TP492	2E		
P547	2H	R486	1I	TP704	3E		
P548	2I	R491	2E	TP748	2A		
P580	1F	R492	2E	TP764	2I		
P746	2D	R494	1J	TP774	4C		
P752	1B	R495	1I				
P754	1B	R502	1I	U102	2B		

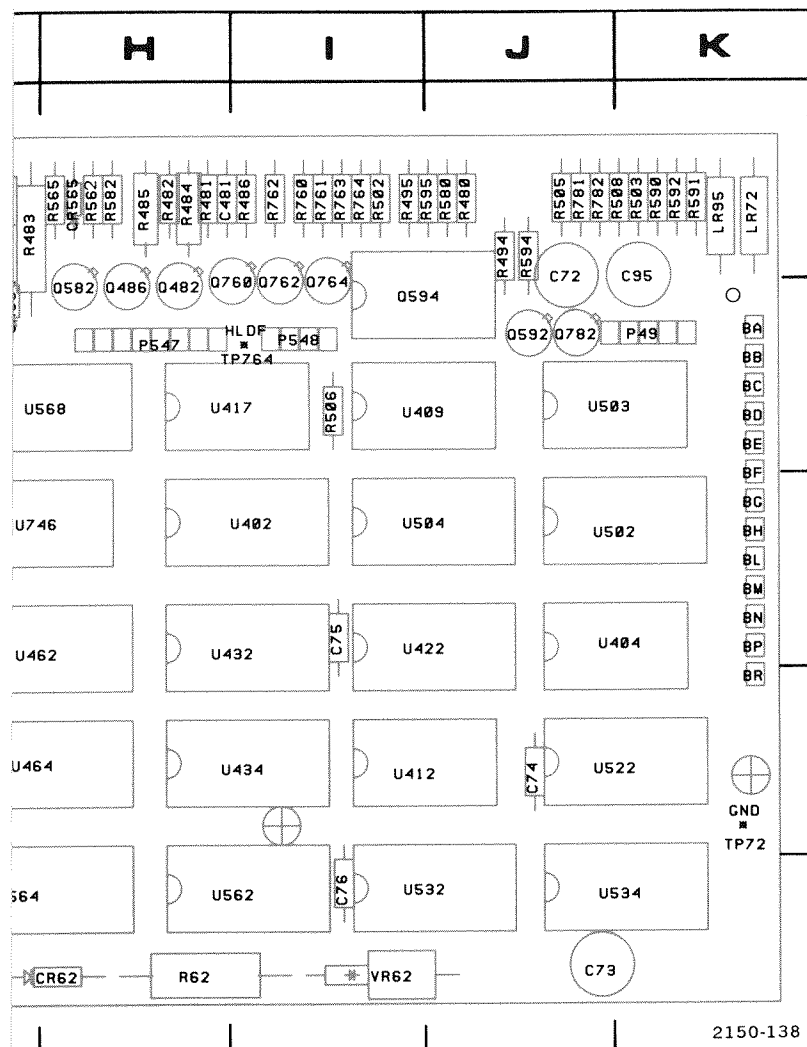

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
C72	1J	Q141	5C	R503	1K	U110	4C
C73	5J	Q151	5A	R505	1J	U132	5E
C74	4J	Q184	5E	R506	2I	U138	5G
C75	3I	Q188	5E	R508	1K	U152	3B
C76	5I	Q202	5C	R562	1H	U156	3D
C77	5G	Q206	5C	R563	2F	U158	4D
C78	4F	Q472	2F	R564	2G	U162	3B
C79	3E	Q482	2H	R565	1H	U172	4A
C93	1D	Q486	2H	R566	1G	U182	4B
C95	1K	Q572	2G	R567	2F	U402	3I
C96	4E	Q582	2H	R569	2F	U404	3K
C97	3D	Q586	2G	R571	1G	U409	2I
C98	3C	Q592	2I	R572	2G	U412	4I
C99	1C	Q594	2I	R580	1J	U415	3E
C187	5E	Q752	1E	R581	1G	U417	2I
C206	5B	Q754	2E	R582	1H	U422	3I
C467	2E	Q756	1C	R583	1G	U432	3I
C468	2F	Q760	2I	R584	1G	U434	4I
C470	2E	Q762	2I	R585	2F	U452	3E
C472	2F	Q764	2I	R586	1G	U454	3E
C481	1H	Q770	2D	R590	1K	U462	3G
C492	2E	Q772	2E	R591	1K	U464	4H
C493	2F	Q774	2D	R592	1K	U468	2F
C494	1F	Q782	2I	R594	1J	U492	2D
C567	2F	Q792	2E	R595	1J	U502	3K
C568	2F	Q796	2E	R704	1B	U503	2I
C570	2F			R705	1B	U504	3I
C572	2G	R62	5H	R736	2C	U522	4K
C581	1G	R141	5D	R737	1E	U532	5I
C583	1G	R142	5C	R748	1A	U534	5J
C704	1B	R150	3B	R749	1A	U552	4G
C705	1B	R151	5A	R751	1D	U554	4E
C748	1A	R152	5A	R752	1E	U562	5I
C749	1A	R156	5D	R753	1E	U564	5G
		R184	5E	R754	2F	U568	2H
CR62	5H	R187	5E	R756	1C	U704	2B
CR151	3B	R188	5D	R757	1C	U714	2C
CR152	3A	R201	5B	R760	1I	U724	3E
CR471	2F	R202	3B	R761	1I	U735	3D
CR564	2G	R203	5C	R762	1I	U738	3D
CR565	1H	R204	5B	R763	1I	U746	3G
CR571	1F	R205	5B	R764	1I	U748	2B
		R206	3B	R770	1D	U752	2C
L73	1E	R463	2E	R771	1D	U756	2B
L704	1B	R467	2E	R772	1D		
		R469	2E	R773	1D	VR62	5I
LR72	1K	R470	1E	R774	1D		
LR95	1K	R471	1F	R781	1J	Y704	1A
		R472	2F	R790	1C		
		R480	1J	R791	1D		
P49	2K	R481	1H	R792	1E		
P141	5E	R482	1H				
P142	5D	R483	1G	TP70	3A		
P145	3D	R484	1H	TP72	4K		
P163	5C	R485	1H	TP492	2E		
P174	5B	R486	1I	TP704	3E		
P547	2H	R491	2E	TP748	2A		
P548	2I	R492	2E	TP764	2I		
P580	1F	R494	1J	TP774	4C		
P746	2D						
P752	1B						
P754	1B						


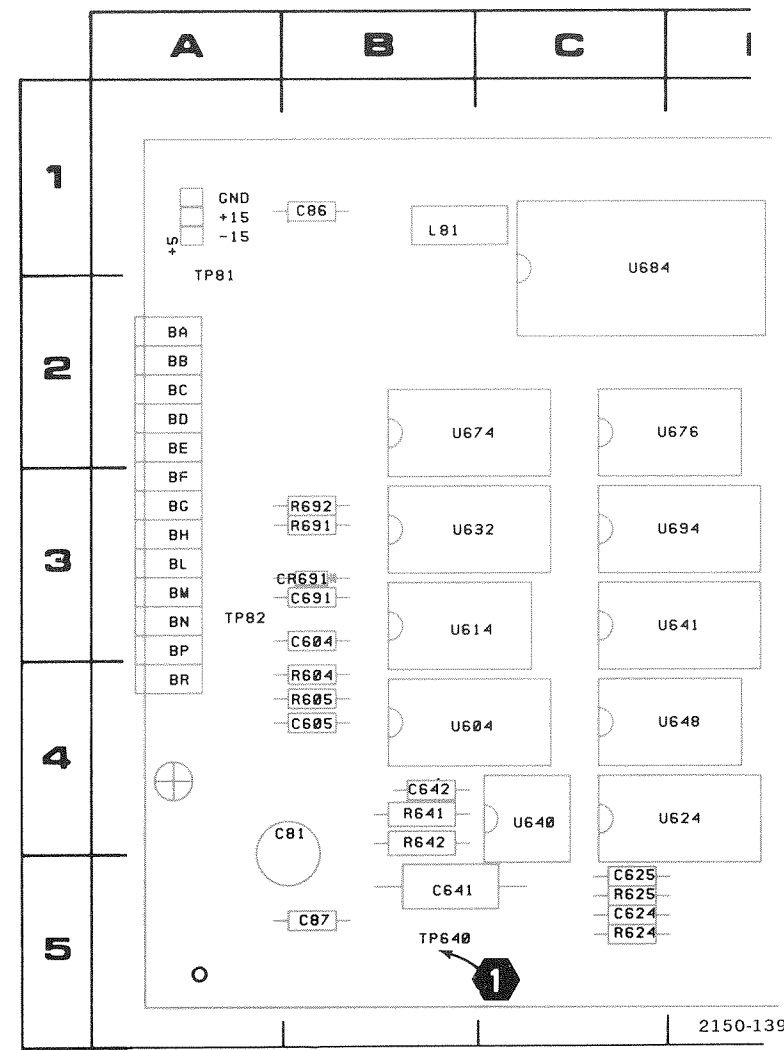


Figure 8-11. Partial A3-Intelligence circuit board. Component locations as viewed from the component side of the board.

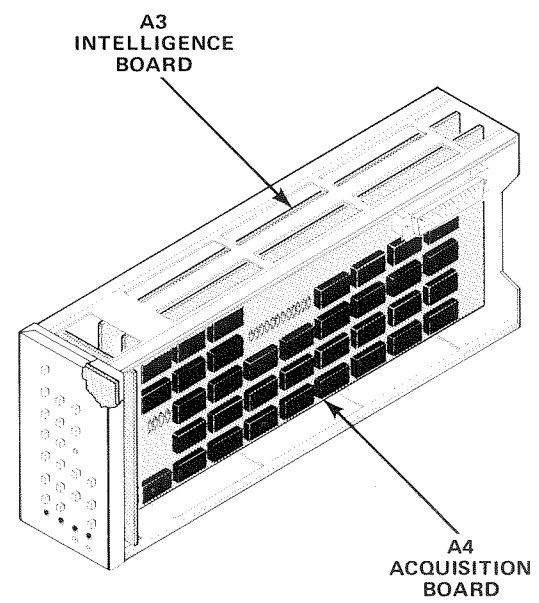



CKT NO	GRID COORD	CKT NO	GRID COORD
C625	5C	U614	3C
C641	5B	U624	4D
C642	4B	U640	4C
		U641	3D
		U642	2E
R625	5C	U648	4D


VOLTAGE AND WAVEFORM CONDITIONS

Voltages and waveforms shown are typical, but may vary between instruments.

TEST SETUP: The 7D01 is connected to the 7000-series mainframe Right-Vertical and A-Horizontal compartments through two 067-0616-00 Flexible Plug-in Extenders. The DF1 is connected to the 7D01 through a 067-0805-00 Cable Extender. The DF1 is set for a STATE TABLE BINARY, 7D01 ONLY display.

The test oscilloscope is dc coupled and internally triggered.

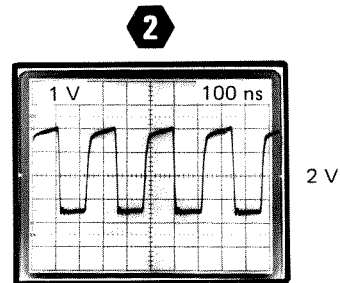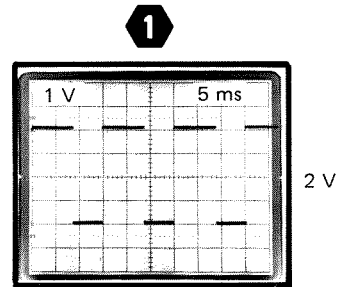

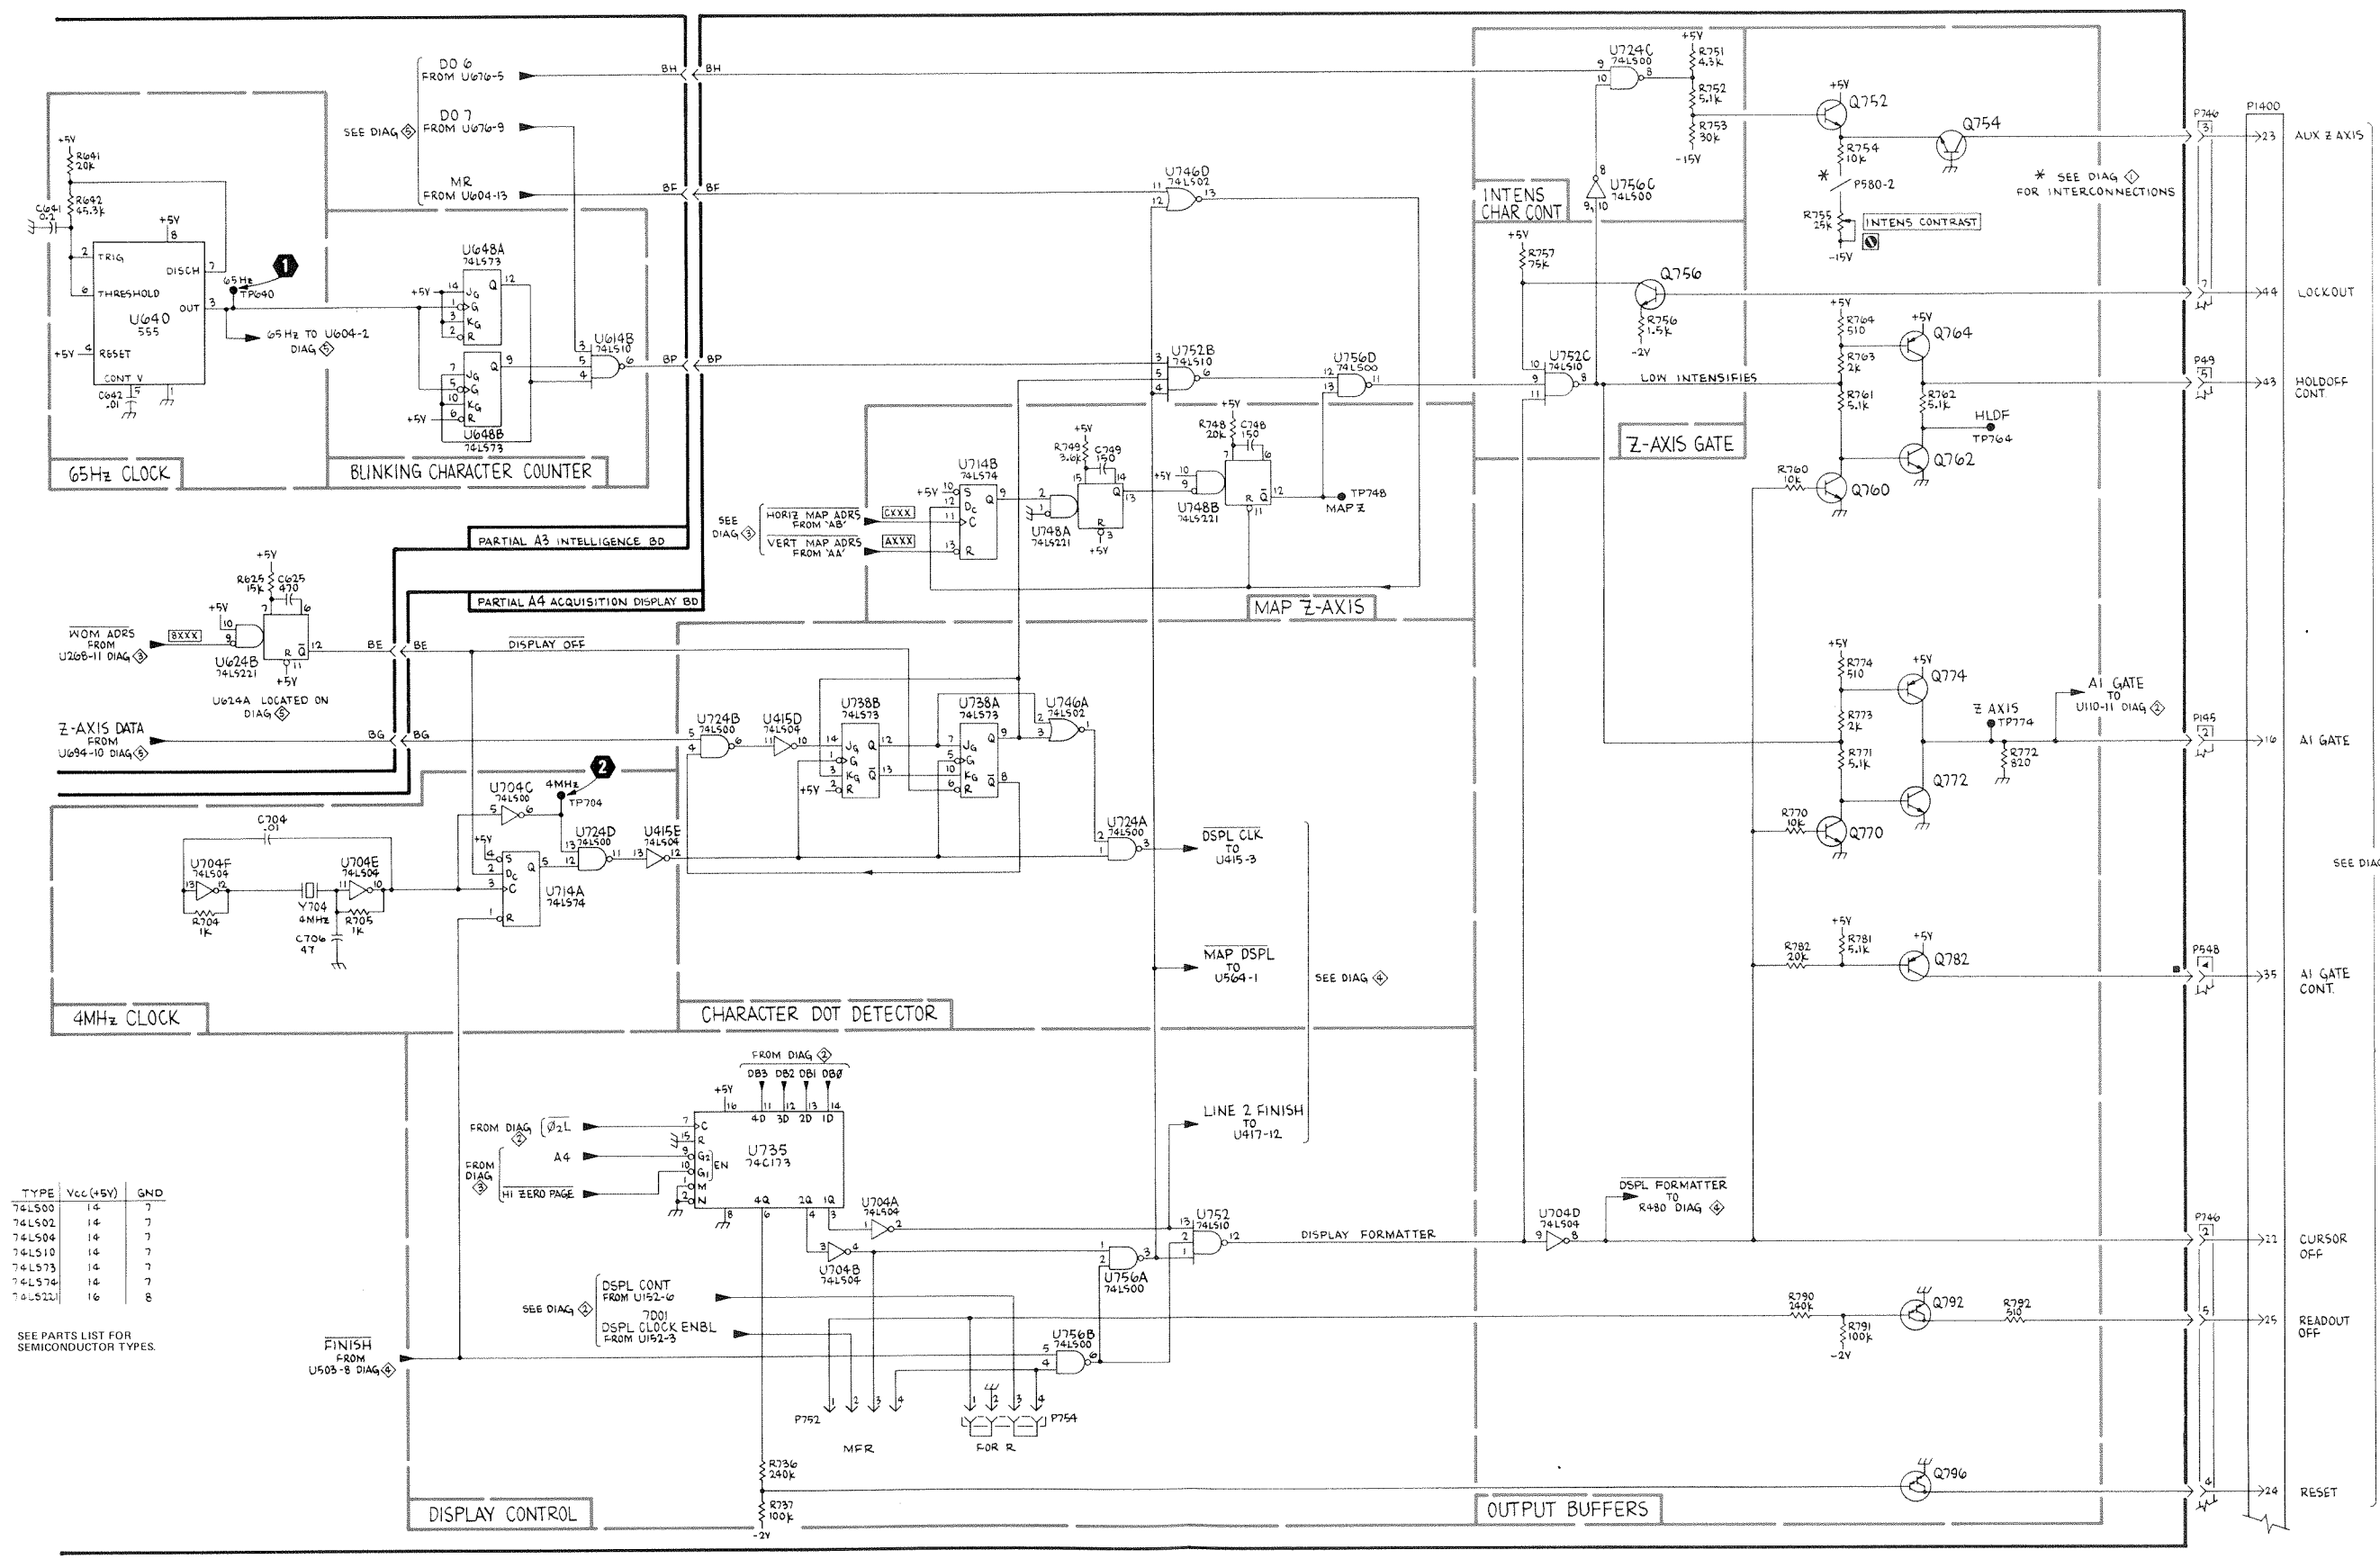

TYPE	Vcc(+5V)	GND
74LS00	14	7
74LS02	14	7
74LS04	14	7
74LS10	14	7
74LS14	14	7
74LS15	14	7
74LS16	14	7
74LS21	16	8

SEE PARTS LIST FOR SEMICONDUCTOR TYPES.



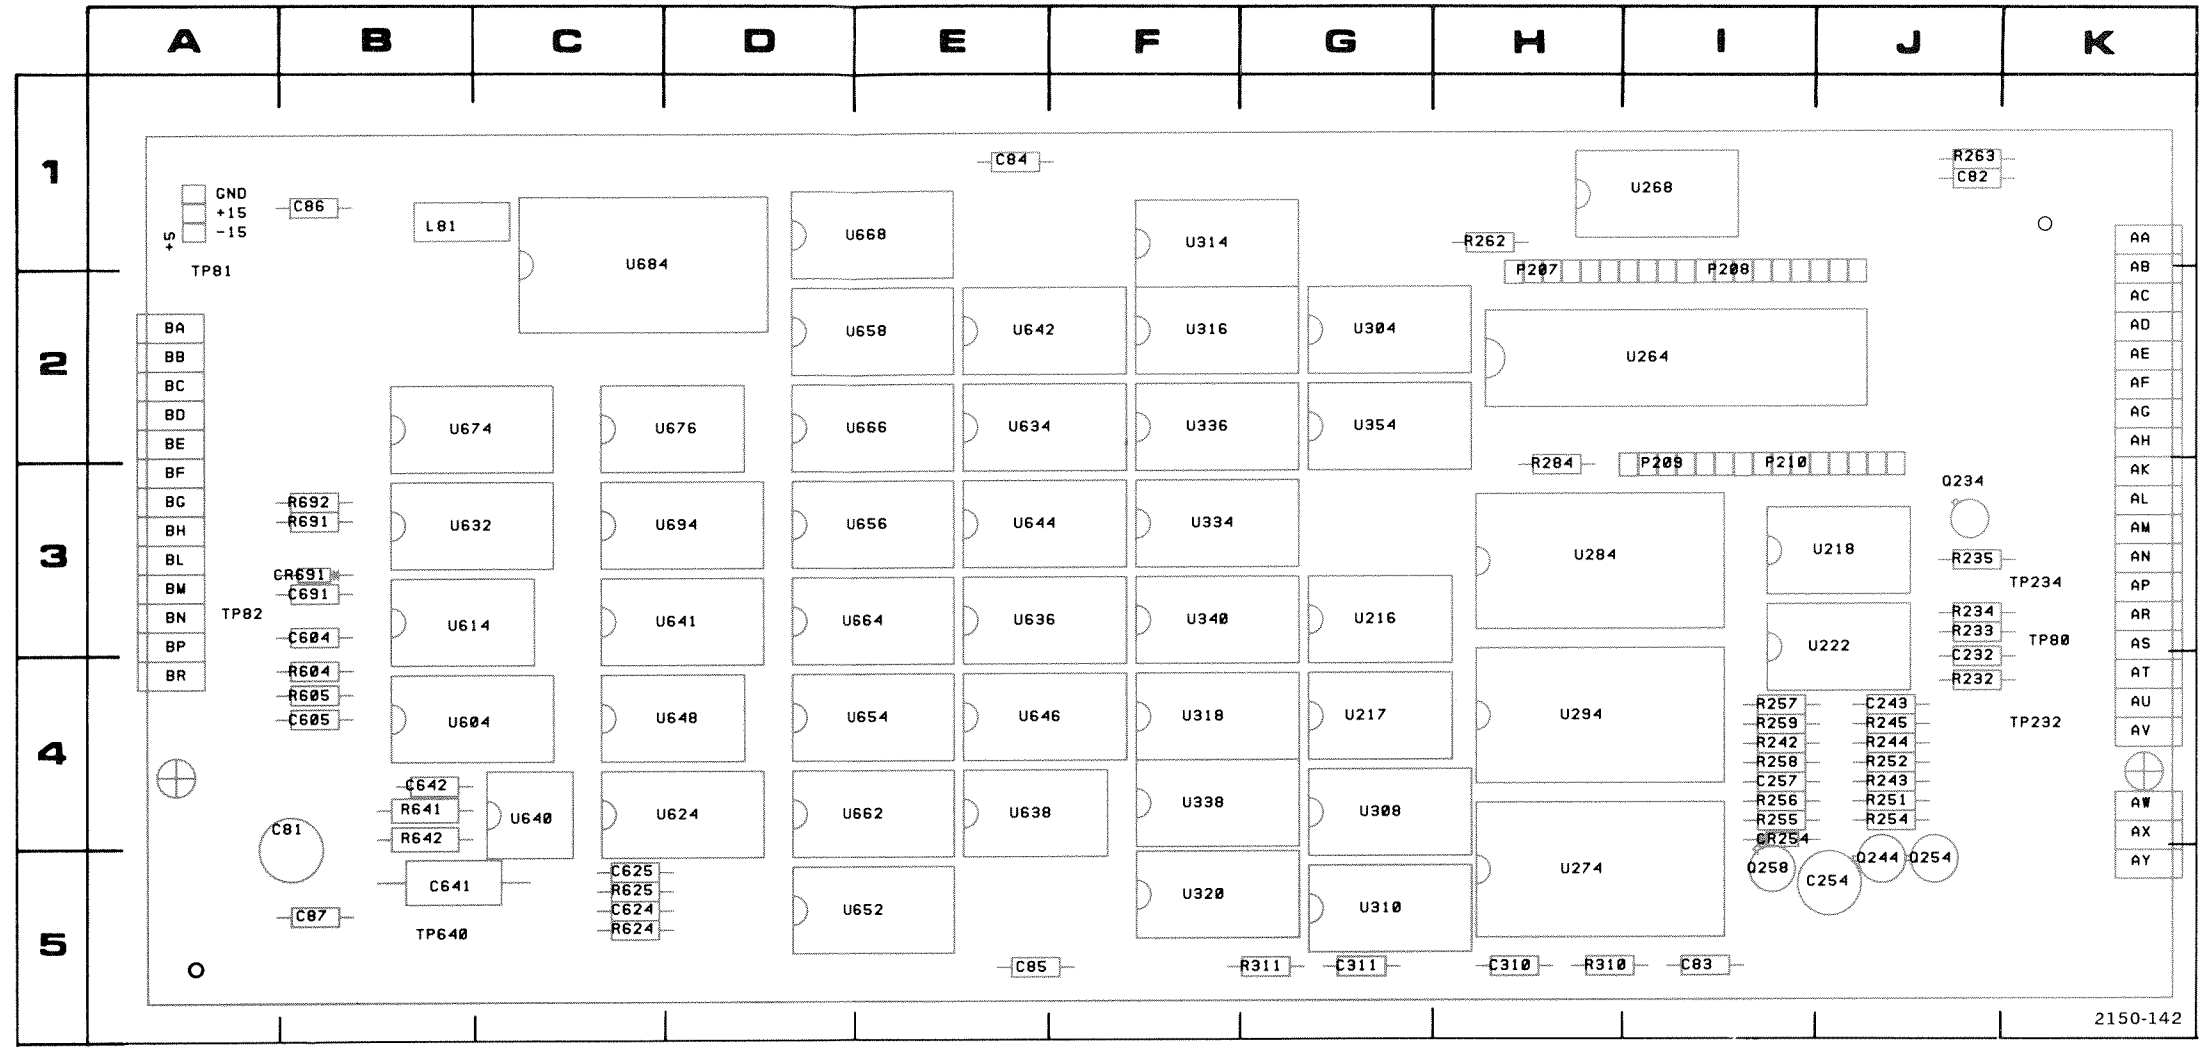


Figure 8-13. Partial A3—Intelligence circuit board component locations.

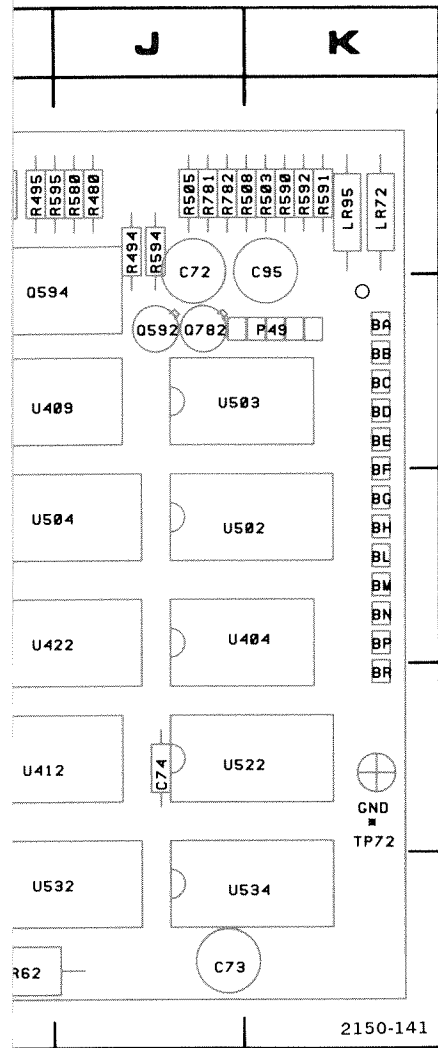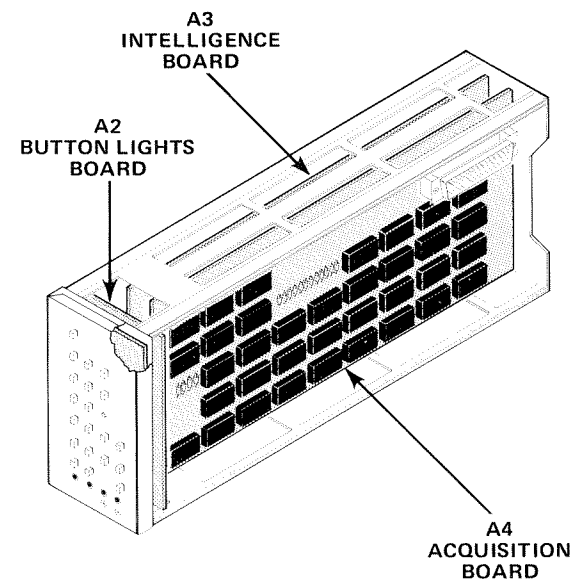

CKT NO	GRID COORD	CKT NO	GRID COORD
C81	4B	C87	5B
C82	1J	L81	1B
C83	5I	TP81	1A
C84	1E	TP82	3A
C85	5E		
C86	1B		


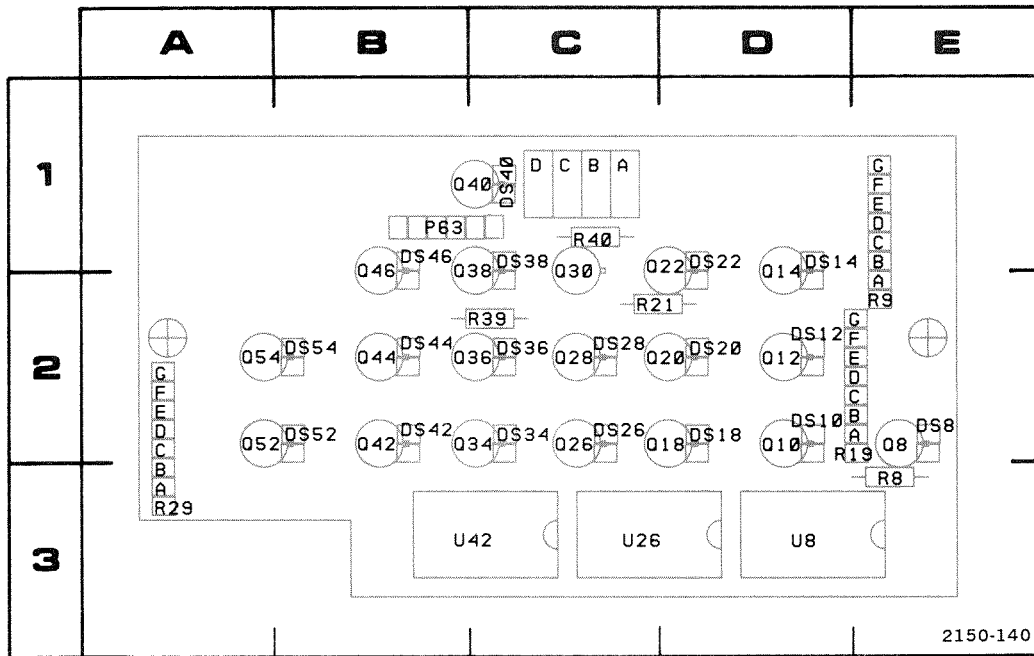


Figure 8-14. A2-Button Lights circuit board component locations, as viewed from component side of the board.

CKT NO	GRID COORD	CKT NO	GRID COORD	CKT NO	GRID COORD
DS8	2E	P63	1B	Q46	1B
DS10	2D	Q8	2E	Q52	2A
DS12	2D	Q10	2D	Q54	2A
DS14	1D	Q12	2D	R8	3E
DS18	2D	Q14	1D	R9	2E
DS20	2D	Q18	2C	R19	2E
DS22	1D	Q20	2C	R21	2C
DS26	2C	Q22	1D	R29	3A
DS28	2C	Q26	2C	R39	2C
DS34	2C	Q28	2C	R40	1C
DS36	2C	Q30	1C		
DS38	1C	Q34	2B	U8	3D
DS40	1C	Q36	2B	U26	3C
DS42	2B	Q38	1B	U42	3C
DS44	2B	Q40	1C		
DS46	1B	Q42	2B		
DS52	2B	Q44	2B		
DS54	2B				



INTERCONNECTIONS

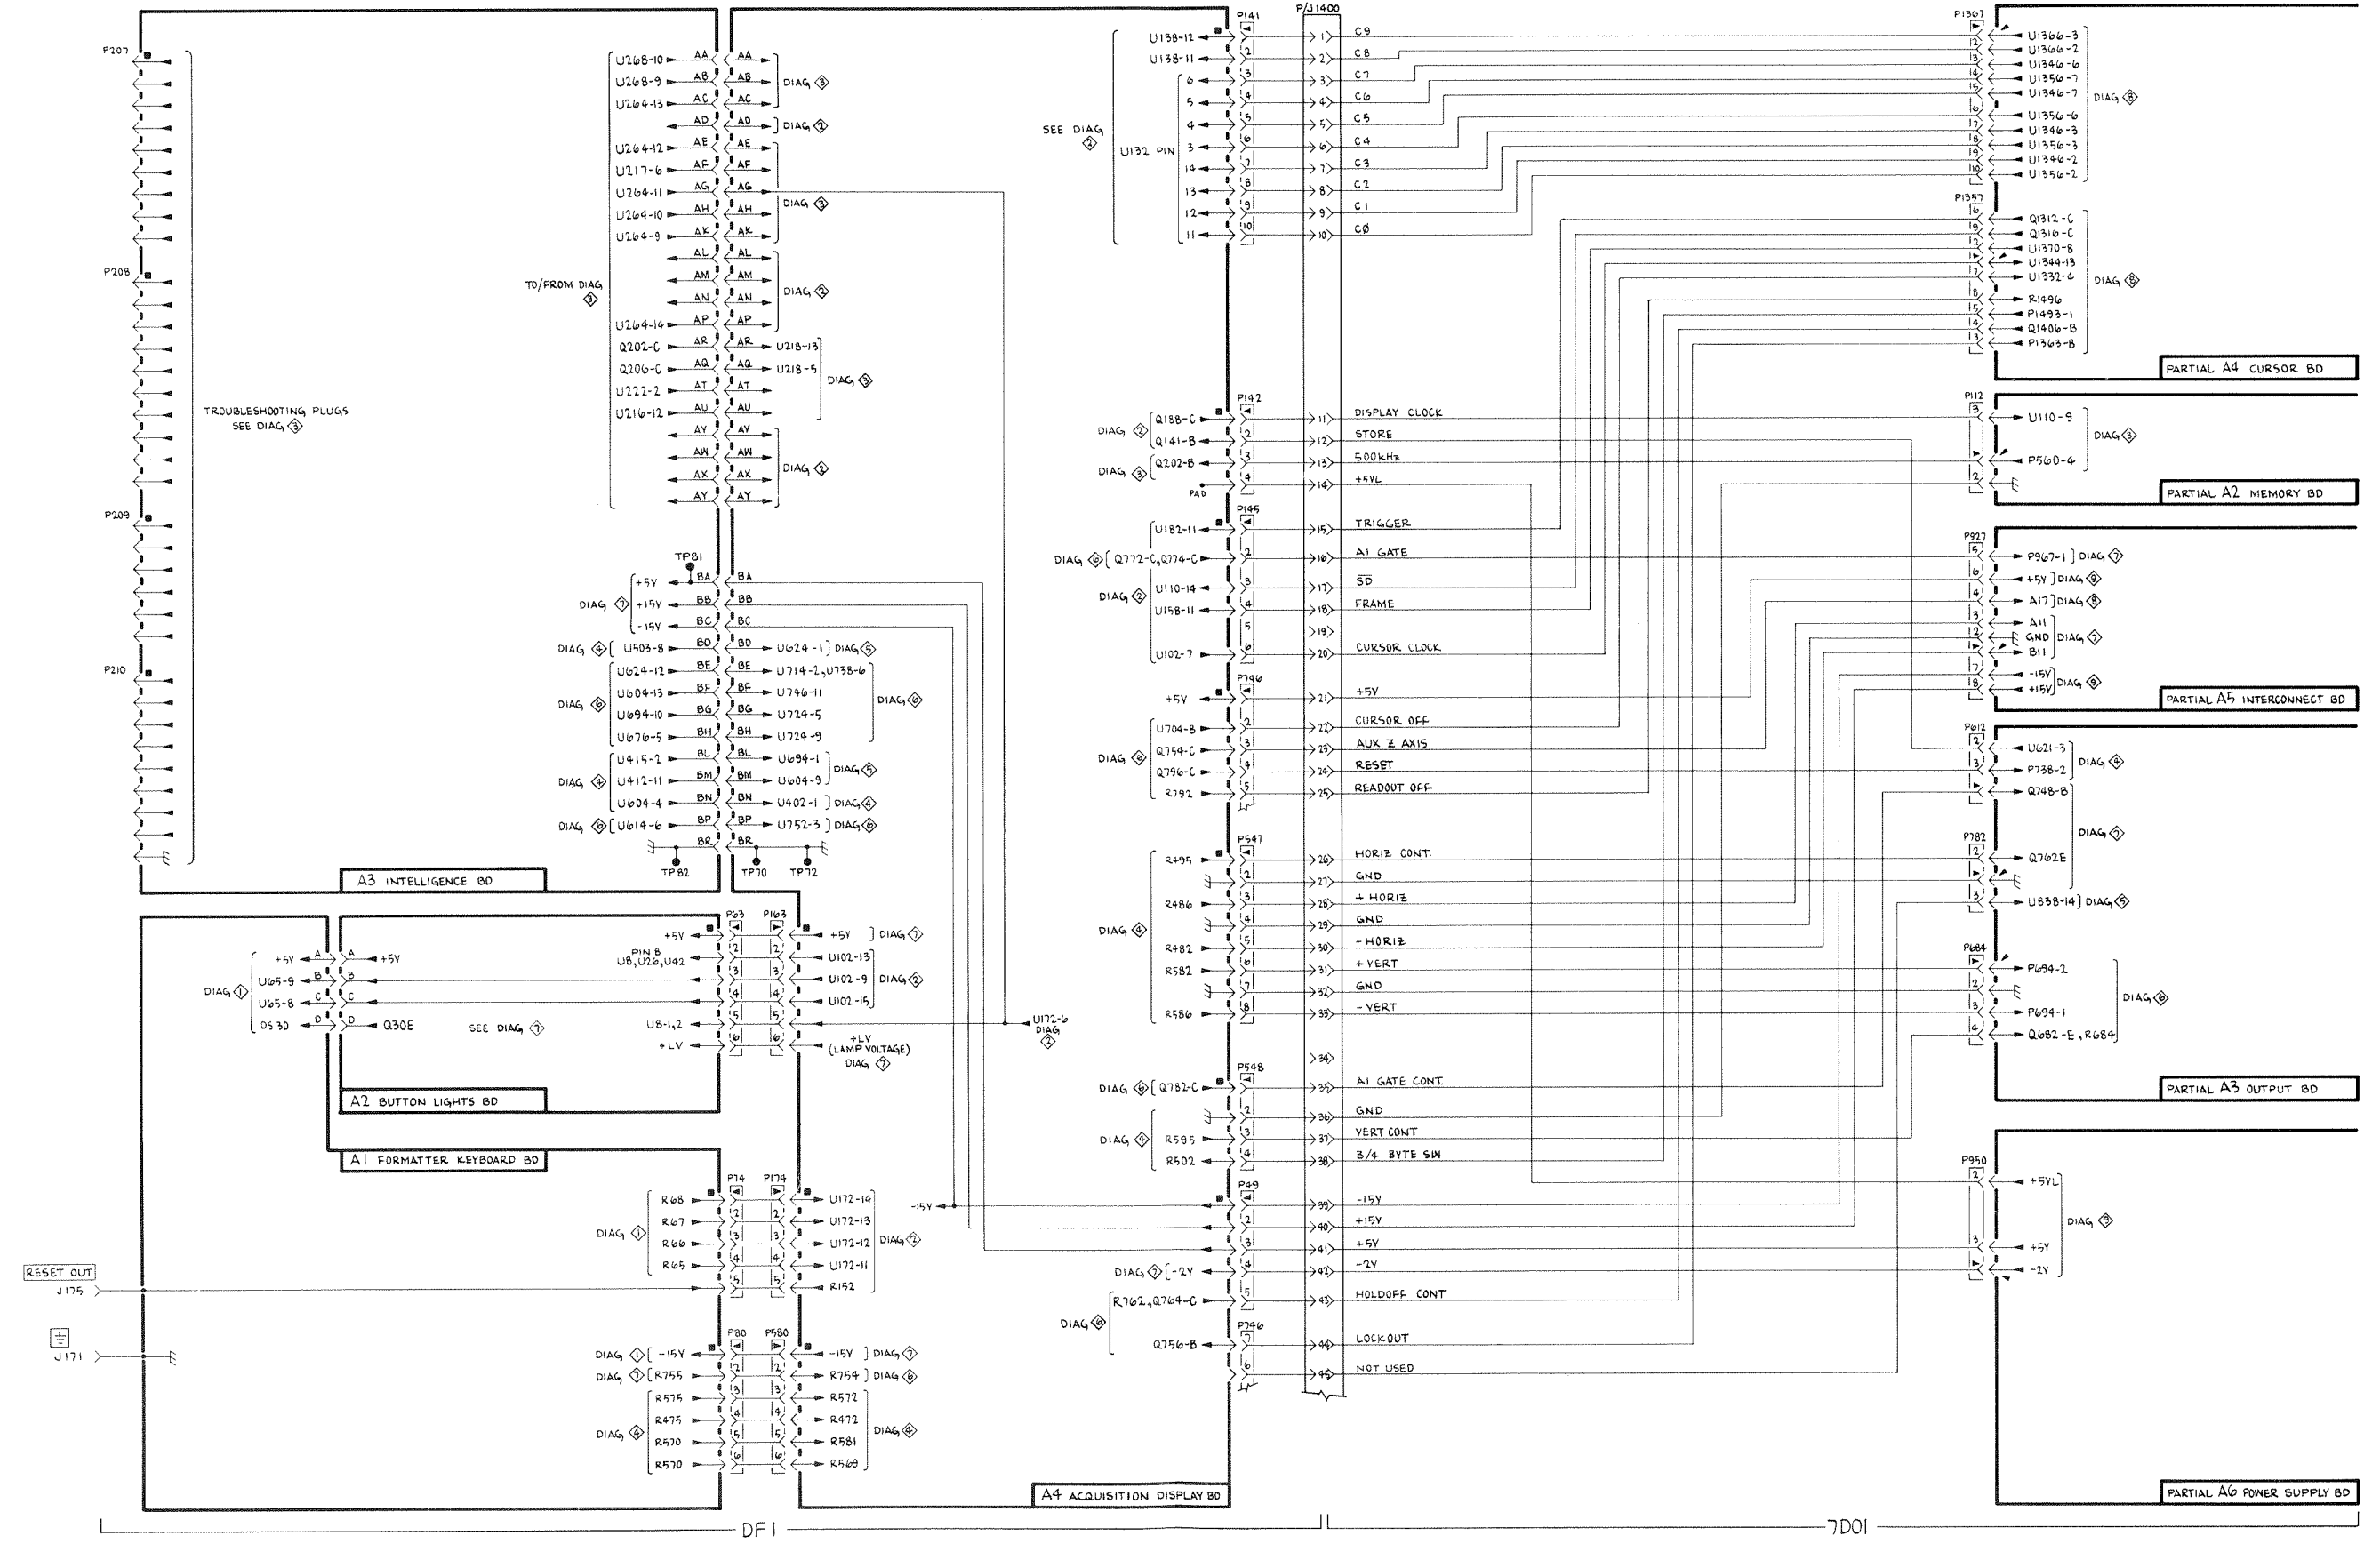

DF 1

INTERCONNECTIONS



REPLACEABLE MECHANICAL PARTS

PARTS ORDERING INFORMATION

Replacement parts are available from or through your local Tektronix, Inc. Field Office or representative.

Changes to Tektronix instruments are sometimes made to accommodate improved components as they become available, and to give you the benefit of the latest circuit improvements developed in our engineering department. It is therefore important, when ordering parts, to include the following information in your order: Part number, instrument type or number, serial number, and modification number if applicable.

If a part you have ordered has been replaced with a new or improved part, your local Tektronix, Inc. Field Office or representative will contact you concerning any change in part number.

Change information, if any, is located at the rear of this manual.

SPECIAL NOTES AND SYMBOLS

X000 Part first added at this serial number

00X Part removed after this serial number

FIGURE AND INDEX NUMBERS

Items in this section are referenced by figure and index numbers to the illustrations.

INDENTATION SYSTEM

This mechanical parts list is indented to indicate item relationships. Following is an example of the indentation system used in the description column.

1 2 3 4 5 *Name & Description*

Assembly and/or Component

Attaching parts for Assembly and/or Component

--- * ---

Detail Part of Assembly and/or Component

Attaching parts for Detail Part

--- * ---

Parts of Detail Part

Attaching parts for Parts of Detail Part

--- * ---

Attaching Parts always appear in the same indentation as the item it mounts, while the detail parts are indented to the right. Indented items are part of, and included with, the next higher indentation. The separation symbol --- * --- indicates the end of attaching parts.

Attaching parts must be purchased separately, unless otherwise specified.

ITEM NAME

In the Parts List, an Item Name is separated from the description by a colon (:). Because of space limitations, an Item Name may sometimes appear as incomplete. For further Item Name identification, the U.S. Federal Cataloging Handbook H6-1 can be utilized where possible.

ABBREVIATIONS

..	INCH	ELCTRN	ELECTRON	IN	INCH	SE	SINGLE END
#	NUMBER SIZE	ELEC	ELECTRICAL	INCAND	INCANDESCENT	SECT	SECTION
ACTR	ACTUATOR	ELCTLT	ELECTROLYTIC	INSUL	INSULATOR	SEMICOND	SEMICONDUCTOR
ADPTR	ADAPTER	ELEM	ELEMENT	INTL	INTERNAL	SHLD	SHIELD
ALIGN	ALIGNMENT	EPL	ELECTRICAL PARTS LIST	LPHLDR	LAMPHOLDER	SHLDR	SHOULDERED
AL	ALUMINUM	EQPT	EQUIPMENT	MACH	MACHINE	SKT	SOCKET
ASSEM	ASSEMBLED	EXT	EXTERNAL	MECH	MECHANICAL	SL	SLIDE
ASSY	ASSEMBLY	FIL	FILLISTER HEAD	MTG	MOUNTING	SLFLKG	SELF-LOCKING
ATTEN	ATTENUATOR	FLEX	FLEXIBLE	NIP	NIPPLE	SLVG	SLEEVING
AWG	AMERICAN WIRE GAGE	FLH	FLAT HEAD	NON WIRE	NOT WIRE WOUND	SPR	SPRING
BD	BOARD	FLTR	FILTER	OBD	ORDER BY DESCRIPTION	SQ	SQUARE
BRKT	BRACKET	FR	FRAME or FRONT	OD	OUTSIDE DIAMETER	SST	STAINLESS STEEL
BRS	BRASS	FSTNR	FASTENER	OVH	OVAL HEAD	STL	STEEL
BRZ	BRONZE	FT	FOOT	PH BRZ	PHOSPHOR BRONZE	SW	SWITCH
BSHG	BUSHING	FXD	FIXED	PL	PLAIN or PLATE	T	TUBE
CAB	CABINET	GSKT	GASKET	PLSTC	PLASTIC	TERM	TERMINAL
CAP	CAPACITOR	HDL	HANDLE	PN	PART NUMBER	THD	THREAD
CER	CERAMIC	HEX	HEXAGON	PNH	PAN HEAD	THK	THICK
CHAS	CHASSIS	HEX HD	HEXAGONAL HEAD	PWR	POWER	TNSN	TENSION
CKT	CIRCUIT	HEX SOC	HEXAGONAL SOCKET	RCPT	RECEPTACLE	TPG	TAPPING
COMP	COMPOSITION	HLCP	HELICAL COMPRESSION	RES	RESISTOR	TRH	TRUSS HEAD
CONN	CONNECTOR	HLEXT	HELICAL EXTENSION	RGD	RIGID	V	VOLTAGE
COV	COVER	HV	HIGH VOLTAGE	RLF	RELIEF	VAR	VARIABLE
CPLG	COUPLING	IC	INTEGRATED CIRCUIT	RTNR	RETAINER	W/	WITH
CRT	CATHODE RAY TUBE	ID	INSIDE DIAMETER	SCH	SOCKET HEAD	WSHR	WASHER
DEG	DEGREE	IDENT	IDENTIFICATION	SCOPE	OSCILLOSCOPE	XFMR	TRANSFORMER
DWR	DRAWER	IMPLR	IMPELLER	SCR	SCREW	XSTR	TRANSISTOR

Replaceable Mechanical Parts—DF1

CROSS INDEX—MFR. CODE NUMBER TO MANUFACTURER

Mfr. Code	Manufacturer	Address	City, State, Zip
01295	TEXAS INSTRUMENTS, INC., SEMICONDUCTOR GROUP	P O BOX 5012, 13500 N CENTRAL EXPRESSWAY	DALLAS, TX 75222
06540	AMATOM ELECTRONIC HARDWARE, DIV. OF MITE CORP.	446 BLAKE ST.	NEW HAVEN, CT 06515
22526	BERG ELECTRONICS, INC.	YOUK EXPRESSWAY	NEW CUMBERLAND, PA 17070
59730	THOMAS AND BETTS COMPANY	36 BUTLER ST.	ELIZABETH, NJ 07207
71279	CAMBRIDGE THERMIONIC CORP.	445 CONCORD AVE.	CAMBRIDGE, MA 02138
71468	ITT CANNON ELECTRIC	666 E. DYER RD.	SANTA ANA, CA 92702
73803	TEXAS INSTRUMENTS, INC., METALLURGICAL MATERIALS DIV.	34 FOREST STREET	ATTLEBORO, MA 02703
80009	TEKTRONIX, INC.	P. O. BOX 500	BEAVERTON, OR 97077
82647	TEXAS INSTRUMENTS, INC., CONTROL PRODUCTS DIV.	34 FOREST ST.	ATTLEBORO, MA 02703
83385	CENTRAL SCREW CO.	2530 CRESCENT DR.	BROADVIEW, IL 60153
87308	N. L. INDUSTRIES, INC., SOUTHERN SCREW DIV.	P. O. BOX 1360	STATESVILLE, NC 28677

Replaceable Mechanical Parts—DF1

Fig. & Index No.	Tektronix Part No.	Serial/Model No. Eff Dscont	Qty	1 2 3 4 5	Name & Description	Mfr Code	Mfr Part Number
1-1	337-1064-04		1		SHIELD,ELEC:RIGHT SIDE	80009	337-1064-00
-2	358-0378-00		4		BUSHING,SLEEVE:GRAY PLASTIC	80009	385-0378-00
-3	333-2236-00		1		PANEL,FRONT:	80009	333-2236-00
-4	348-0235-00		2		SHLD GSKT,ELEC:4.734 INCH LONG	80009	348-0235-00
-5	-----		1		CKT BOARD ASSY:BUTTON LIGHTS(SEE A2 EPL) (ATTACHING PARTS)		
-6	211-0007-00		4		SCREW,MACHINE:4-40 X 0.188 INCH,PNH STL - - - * - - -	83385	OBD
	-----		-		. CKT BOARD ASSY INCLUDES:		
-7	136-0269-02		3		. SOCKET,PLUG-IN:14 CONTACT,LOW CLEARANCE	01295	C931402
-8	136-0263-04		4		. SOCKET,PIN TERM:FOR 0.025 INCH SQUARE PIN	22526	75377-001
-9	131-0608-00		6		. CONTACT,ELEC:0.365 INCH LONG	22526	47357
-10	210-1002-00		4		. WASHER,FLAT:0.125 ID X 0.25 INCH OD,BRS	12327	OBD
-11	-----		1		CKT BOARD ASSY:KEYBOARD(SEE A1 EPL) (ATTACHING PARTS)		
-12	129-0236-00		4		SPACER,POST:0.188 HEX X 0.375 INCH LONG - - - * - - -	06540	9726-A-0440
	-----		-		. CKT BOARD ASSY INCLUDES:		
-13	136-0252-04		14		. SOCKET,PIN TERM:0.188 INCH LON	22526	75060
-14	-----		21		. ACTR ASSY,PB:(SEE S8,S10,S12,S14,S18,S20 - . S22,S26,S28,S34,S36,S38,S40,S42,S44,S46, - . S48,S52,S54,S58 EPL)		
-15	136-0591-00		4		. SOCKET ASSY,CRT:	80009	136-0591-00
-16	131-0608-00		11		. CONTACT,ELEC:0.365 INCH LONG	22526	47357
-17	136-0387-00		1		JACK,TIP:GRAY	71279	450-4352-01-0318
-18	136-0387-01		1		JACK,TIP:BLACK	71279	450-4352-01-0310
-19	386-3632-00		1		SUBPANEL,FRONT: (ATTACHING PARTS)	80009	386-3632-00
-20	213-0192-00		4		SCR,TPG,THD FOR:6-32 X 0.50 INCH,PNH STL - - - * - - -	87308	OBD
-21	-----		1		CKT BOARD ASSY:INTELLIGENCE(SEE A3 EPL) (ATTACHING PARTS)		
-22	211-0007-00		6		SCREW,MACHINE:4-40 X 0.188 INCH,PNH STL - - - * - - -	83385	OBD
	-----		-		. CKT BOARD ASSY INCLUDES:		
-23	136-0252-04		12		. SOCKET,PIN TERM:0.188 INCH LON	22526	75060
-24	136-0263-04		34		. SOCKET,PIN TERM:FOR 0.025 INCH SQUARE PIN	22526	75377-001
-25	214-0579-00		6		. TERM.,TEST PT:0.40 INCH LONG	80009	214-0579-00
-26	131-0608-00		34		. CONTACT,ELEC:0.365 INCH LONG	22526	47357
-27	136-0514-00		1		. SOCKET,PLUG-IN:MICROCIRCUIT,8 CONTACT	01295	C930802
-28	136-0269-02		8		. SOCKET,PLUG-IN:14 CONTACT,LOW CLEARANCE	01295	C931402
-29	136-0260-02		32		. SOCKET,PLUG-IN:16 CONTACT,LOW CLEARANCE	01295	C931602
-30	136-0578-00		4		. SOCKET,PLUG-IN:24 DIP,LOW PROFILE	01295	C932402
-31	136-0623-00		1		. SOCKET,PLUG-IN:40 DIP,LOW PROFILE	73803	C934002
-32	346-0121-00		1		STRAP,ELEC COMP:TIE DOWN,5.0 LONG (ATTACHING PARTS)	59730	T4-34M
-33	211-0507-00		1		SCREW,MACHINE:6-32 X 0.312 INCH,PNH STL - - - * - - -	83385	OBD
-34	385-0127-00		1		SPACER,POST:ALUM HEX,0.25X 0.281 (ATTACHING PARTS)	80009	385-0127-00
-35	211-0503-00		1		SCREW,MACHINE:6-32 X 0.188 INCH,PNH STL - - - * - - -	83385	OBD
-36	-----		1		CKT BOARD ASSY:ACQUISITION(SEE A4 EPL) (ATTACHING PARTS)		
-37	211-0007-00		6		SCREW,MACHINE:4-40 X 0.188 INCH,PNH STL - - - * - - -	83385	OBD
	-----		-		. CKT BOARD ASSY INCLUDES:		
-38	136-0252-04		75		. SOCKET,PIN TERM:0.188 INCH LON	22526	75060
-39	214-0579-00		7		. TERM.,TEST PT:0.40 INCH LONG	80009	214-0579-00
-40	131-0608-00		67		. CONTACT,ELEC:0.365 INCH LONG	22526	47357
-41	131-0592-00		34		. CONTACT,ELEC:0.885 INCH LONG	22526	47353
-42	131-1207-00		1		. LINK,TERM.CONNE:4 WIRE BLACK	80009	131-1207-00
-43	136-0514-00		1		. SOCKET,PLUG-IN:MICROCIRCUIT,8 CONTACT	01295	C930802

Replaceable Mechanical Parts—DF1

Fig. & Index No.	Tektronix Part No.	Serial/Model No. Eff Dscont	Qty	1	2	3	4	5	Name & Description	Mfr Code	Mfr Part Number
1-44	136-0269-02		17	.					SOCKET, PLUG-IN:14 CONTACT, LOW CLEARANCE	01295	C931402
-45	136-0260-02		30	.					SOCKET, PLUG-IN:16 CONTACT, LOW CLEARANCE	01295	C931602
-46	386-3633-00		1						PANEL, REAR: (ATTACHING PARTS)	80009	386-3633-00
-47	213-0192-00		4	SCR, TPG, THD FOR: 6-32 X 0.50 INCH, PNH STL						87308	OBD
-48	179-2505-00		1	WIRING HARNESS: CONNECTOR (ATTACHING PARTS)						80009	179-2505-00
-49	211-0007-00		2	SCREW, MACHINE: 4-40 X 0.188 INCH, PNH STL						83385	OBD
-50	131-1344-00		1	CONNECTOR, PLUG, :50 CONT, MALE D						71468	DD-50P
-51	131-0707-00		78	CONTACT, ELEC: 0.48" L, 22-26 AWG WIRE						22526	47439
-52	352-0169-00		1	CONN BODY, PL, EL: 2 WIRE BLACK						80009	352-0169-00
-53	352-0162-00		1	CONN BODY, PL, EL: 4 WIRE BLACK						80009	352-0162-00
	352-0162-02		1	CONN BODY, PL, EL: 4 WIRE RED						80009	352-0162-02
	352-0162-08		1	CONN BODY, PL, EL: 4 WIRE GRAY						80009	352-0162-08
-54	352-0163-04		2	CONN BODY, PL, EL: 5 WIRE YELLOW						80009	352-0163-04
	352-0163-09		1	CONN BODY, PL, EL: 5 WIRE WHITE						80009	352-0163-09
-55	352-0164-00		1	CONN BODY, PL, EL: 6 WIRE BLACK						80009	352-0164-00
	352-0164-03		2	CONN BODY, PL, EL: 6 WIRE ORANGE						80009	352-0164-03
	352-0164-05		1	CONN BODY, PL, EL: 6 WIRE GREEN						80009	352-0164-05
-56	352-0165-06		1	CONN BODY, PL, EL: 7 WIRE BLUE						80009	352-0165-06
-57	352-0166-07		1	CONN BODY, PL, EL: 8 WIRE VIOLET						80009	352-0166-07
-58	352-0168-01		1	CONN BODY, PL, EL: 10 WIRE BROWN						80009	352-0168-01
-59	220-0790-00		2	NUT, BLOCK: 0.188 X 0.5 INCH SQUARE (ATTACHING PARTS FOR EACH)						80009	220-0790-00
-60	211-0025-00		1	SCREW, MACHINE: 4-40 X 0.375 100 DEG, FLH STL						83385	OBD
-61	214-1337-00		2	PIN, SPRING: 0.10 OD X 0.25 INCH L, STL						80009	214-1337-00
-62	214-2488-00		3	LATCH: GRAY PLASTIC						80009	214-2488-00
-63	214-1061-00		1	SPRING, GROUND: FLAT						80009	214-1061-00
-64	220-0793-00		6	NUT BLOCK: (1) 4-40 THRU, (1) 4-40 CROSS (ATTACHING PARTS FOR EACH)						80009	220-0793-00
-65	211-0105-00		1	SCREW, MACHINE: 4-40 X 0.188" 100 DEG, FLH STL						83385	OBD
-66	426-0505-20		1	FR SECT, PLUG-IN: TOP						80009	426-0505-20
-67	426-0499-20		1	FR SECT, PLUG-IN: BOTTOM						80009	426-0499-20


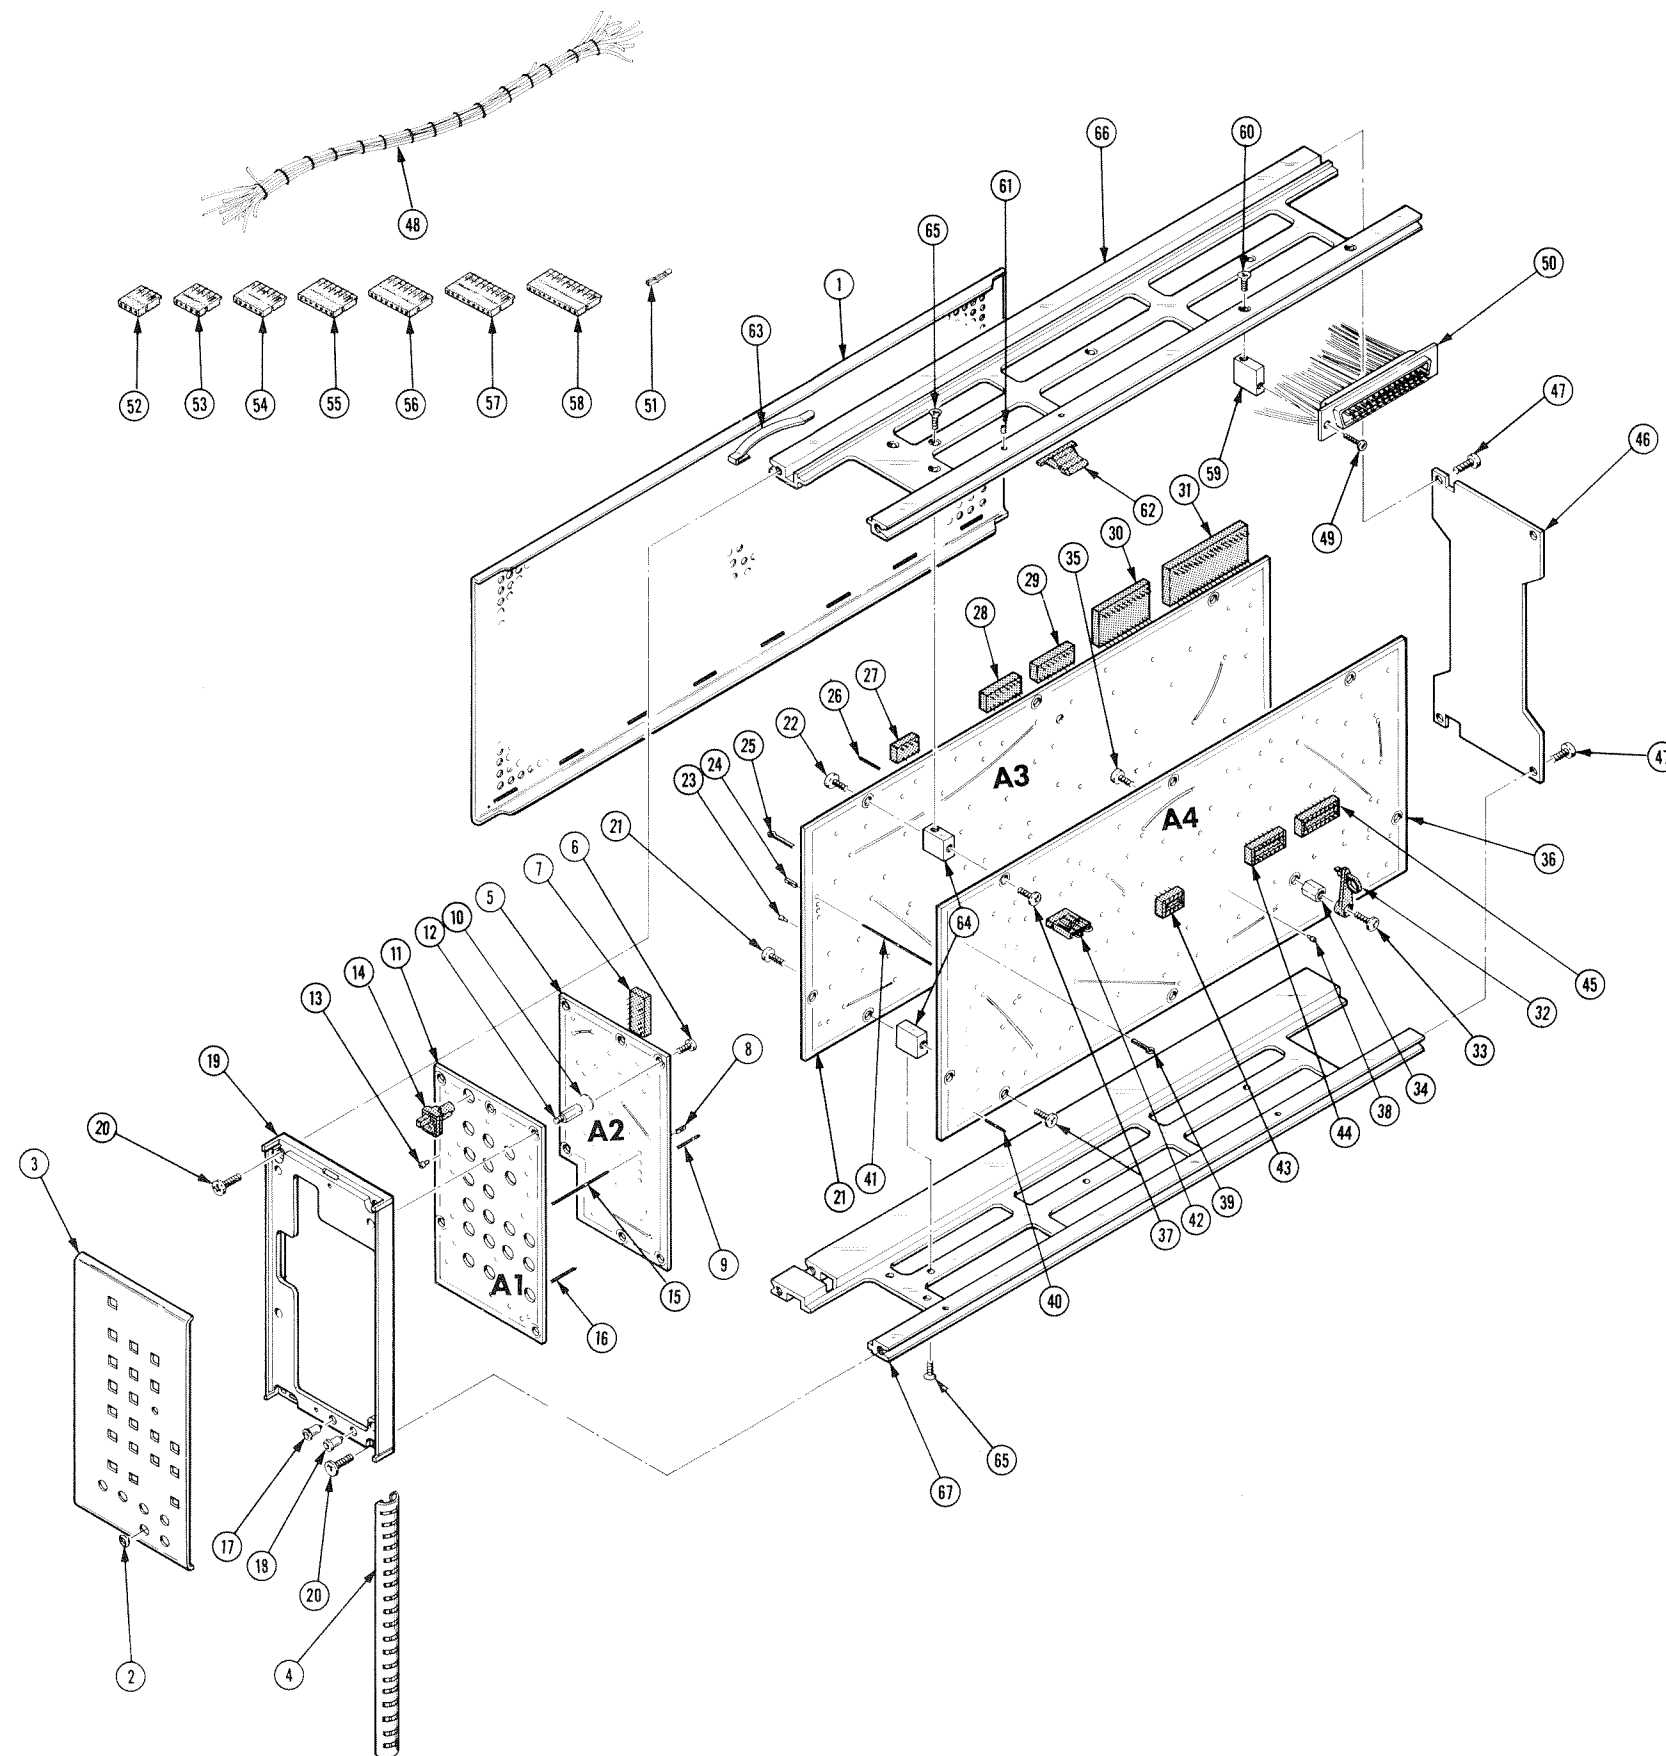


Fig. & Index No.	Tektronix Part No.	Serial/Model No. Eff	Dscont	Qty	1	2	3	4	5	Name & Description	Mfr Code	Mfr Part Number
	070-2149-00			1						MANUAL, TECH: OPERATORS	80009	070-2149-00
	070-2150-00			1						MANUAL, TECH: INSTRUCTION	80009	070-2150-00

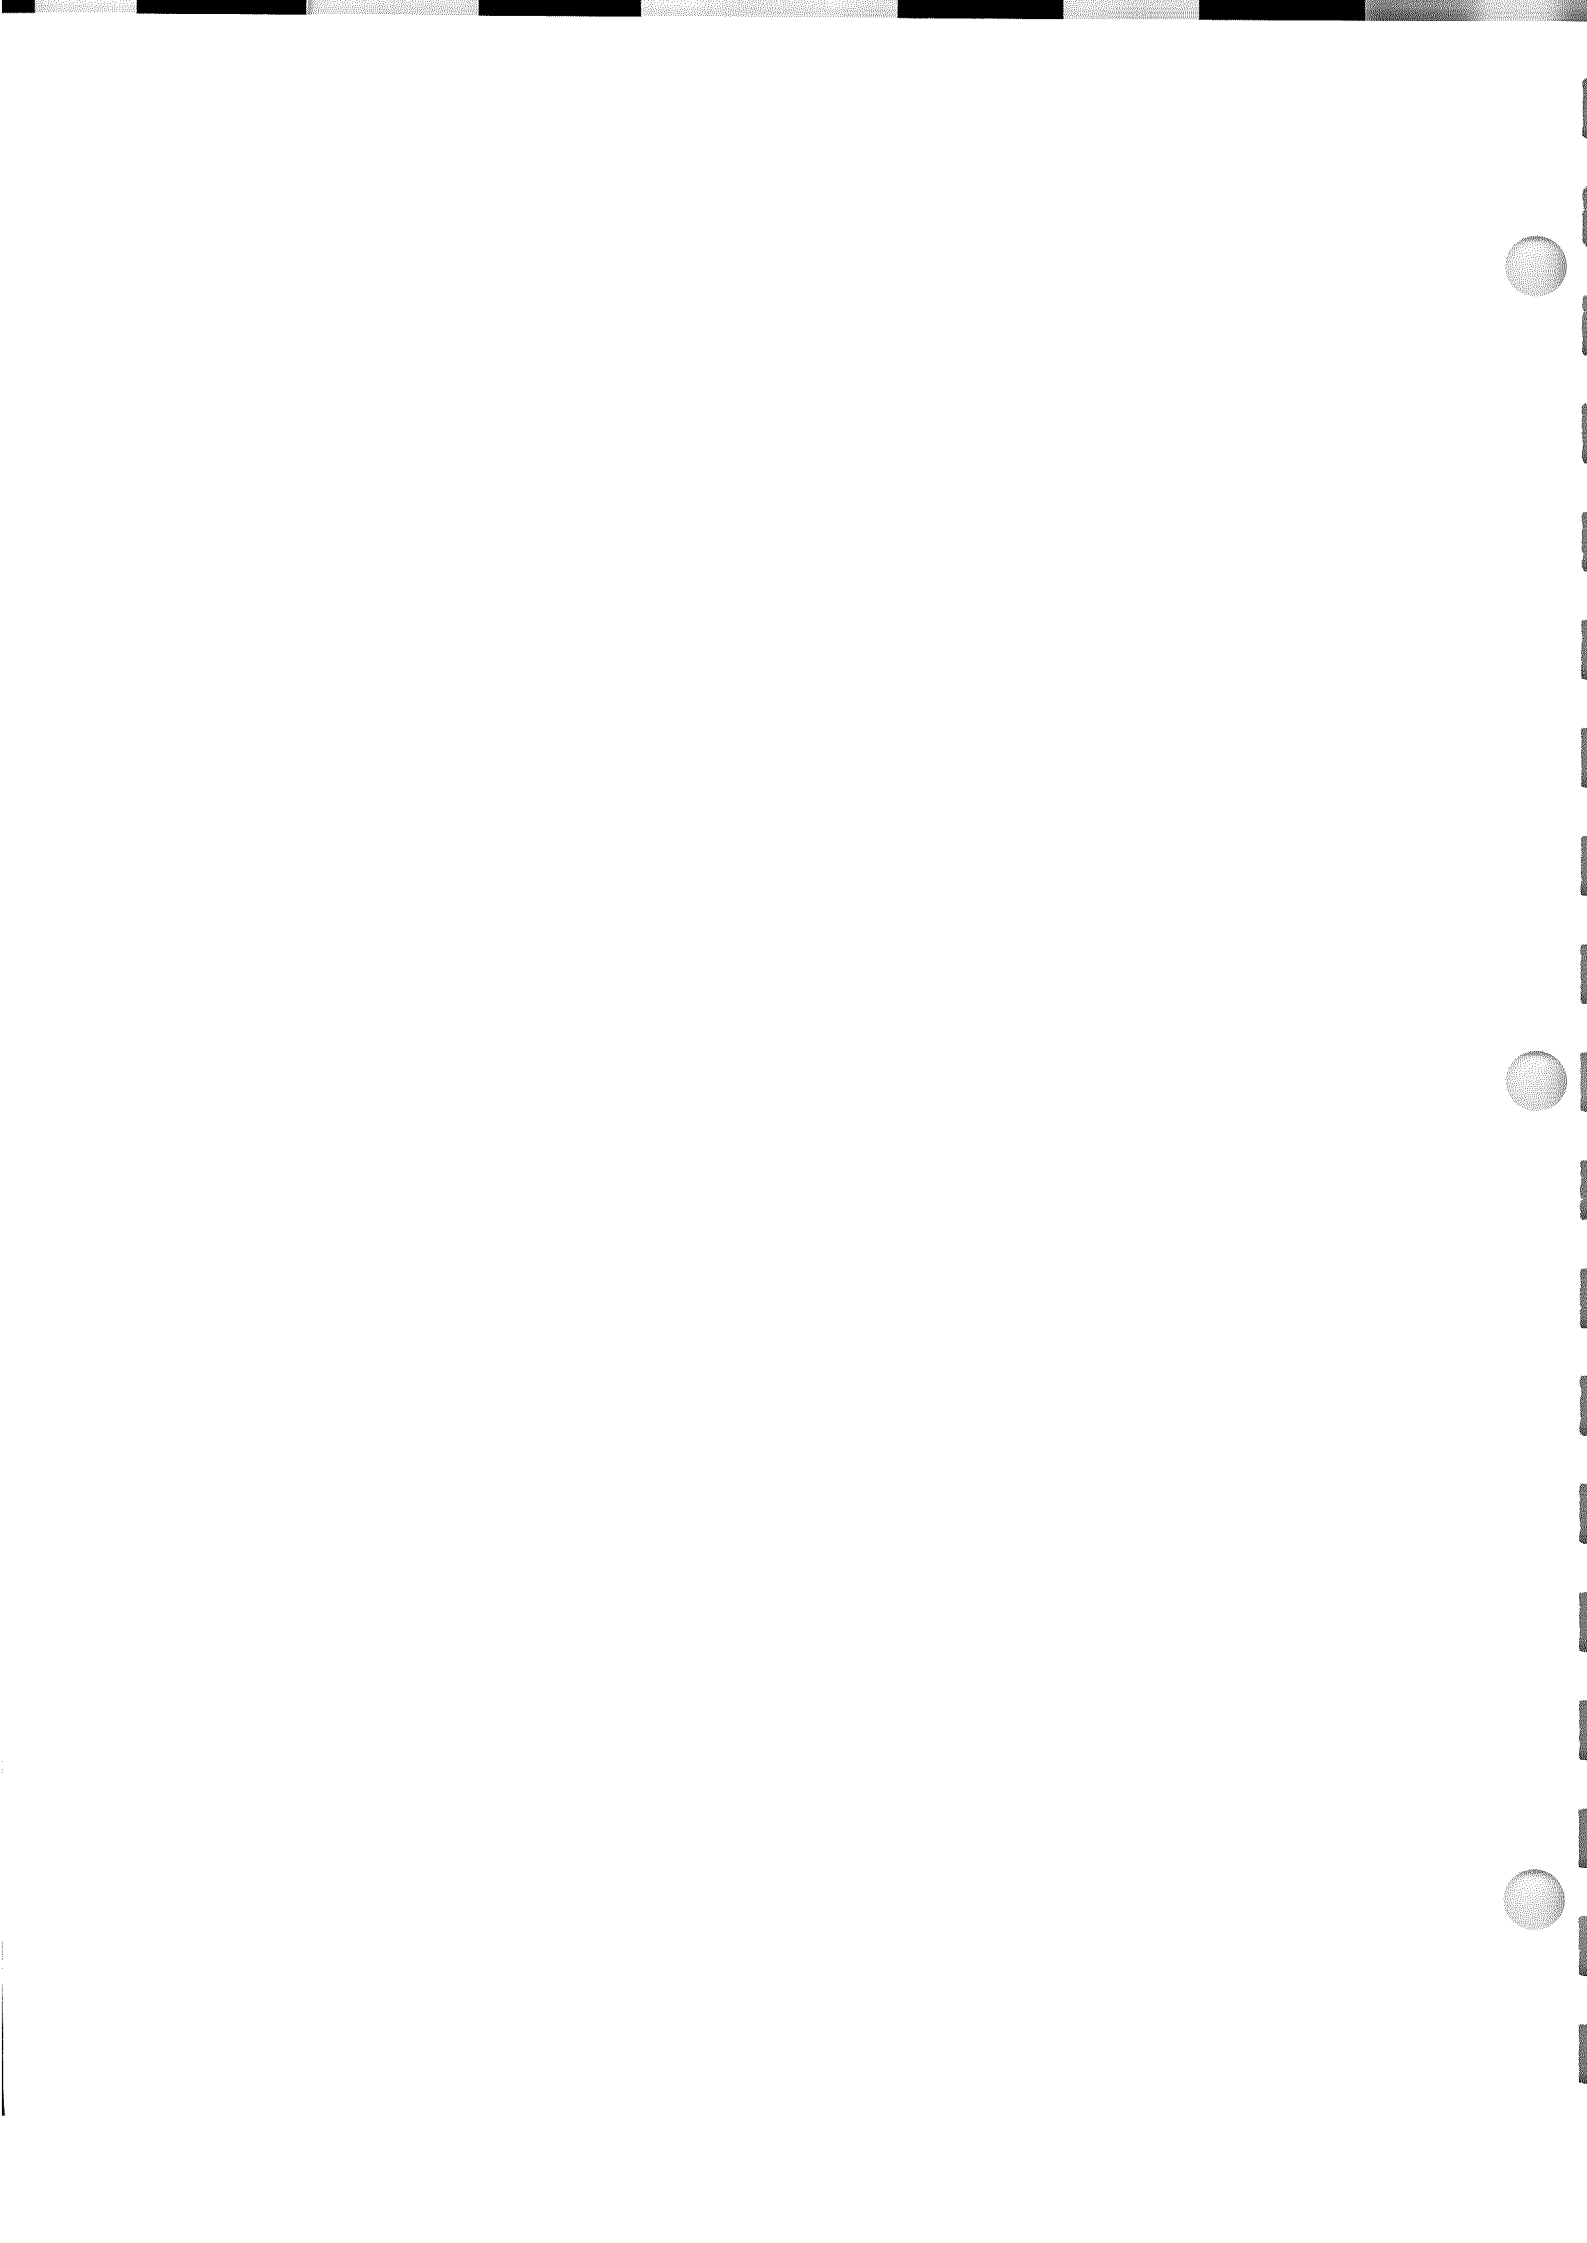

MANUAL CHANGE INFORMATION

At Tektronix, we continually strive to keep up with latest electronic developments by adding circuit and component improvements to our instruments as soon as they are developed and tested.

Sometimes, due to printing and shipping requirements, we can't get these changes immediately into printed manuals. Hence, your manual may contain new change information on following pages.

A single change may affect several sections. Since the change information sheets are carried in the manual until all changes are permanently entered, some duplication may occur. If no such change pages appear following this page, your manual is correct as printed.

SERVICE NOTE

Because of the universal parts procurement problem, some electrical parts in your instrument may be different from those described in the Replaceable Electrical Parts List. The parts used will in no way alter or compromise the performance or reliability of this instrument. They are installed when necessary to ensure prompt delivery to the customer. Order replacement parts from the Replaceable Electrical Parts List.

CALIBRATION TEST EQUIPMENT REPLACEMENT

Calibration Test Equipment Chart

This chart compares TM 500 product performance to that of older Tektronix equipment. Only those characteristics where significant specification differences occur, are listed. In some cases the new instrument may not be a total functional replacement. Additional support instrumentation may be needed or a change in calibration procedure may be necessary.

Comparison of Main Characteristics

DM 501 replaces 7D13		
PG 501 replaces 107	PG 501 - Risetime less than 3.5 ns into 50 Ω .	107 - Risetime less than 3.0 ns into 50 Ω .
108	PG 501 - 5 V output pulse; 3.5 ns Risetime.	108 - 10 V output pulse; 1 ns Risetime.
111	PG 501 - Risetime less than 3.5 ns; 8 ns Pretrigger pulse delay.	111 - Risetime 0.5 ns; 30 to 250 ns Pretrigger Pulse delay.
114	PG 501 - ± 5 V output.	114 - ± 10 V output. Short proof output.
115	PG 501 - Does not have Paired, Burst, Gated, or Delayed pulse mode; ± 5 V dc Offset. Has ± 5 V output.	115 - Paired, Burst, Gated, and Delayed pulse mode; ± 10 V output. Short-proof output.
PG 502 replaces 107	PG 502 - 5 V output	108 - 10 V output.
108	PG 502 - Risetime less than 1 ns; 10 ns Pretrigger pulse delay.	111 - Risetime 0.5 ns; 30 to 250 ns Pretrigger pulse delay.
111	PG 502 - ± 5 V output	114 - ± 10 V output. Short proof output.
114	PG 502 - Does not have Paired, Burst, Gated, Delayed & Undelayed pulse mode; Has ± 5 V output.	115 - Paired, Burst, Gated, Delayed & Undelayed pulse mode; ± 10 V output. Short-proof output.
115	PG 502 - Does not have Paired or Delayed pulse. Has ± 5 V output.	2101 - Paired and Delayed pulse; 10 V output.
2101		
PG 506 replaces 106	PG 506 - Positive-going trigger output signal at least 1 V; High Amplitude output, 60 V.	106 - Positive and Negative-going trigger output signal, 50 ns and 1 V; High Amplitude output, 100 V.
067-0502-01	PG 506 - Does not have chopped feature.	0502-01 - Comparator output can be alternately chopped to a reference voltage.
SG 503 replaces 190, 190A, 190B	SG 503 - Amplitude range 5 mV to 5.5 V p-p.	190B - Amplitude range 40 mV to 10 V p-p.
191	SG 503 - Frequency range 250 kHz to 250 MHz.	191 - Frequency range 350 kHz to 100 MHz.
067-0532-01	SG 503 - Frequency range 250 kHz to 250 MHz.	0532-01 - Frequency range 65 MHz to 500 MHz.
TG 501 replaces 180, 180A	TG 501 - Marker outputs, 5 sec to 1 ns. Sinewave available at 5, 2, and 1 ns. Trigger output - slaved to marker output from 5 sec through 100 ns. One time-mark can be generated at a time.	180A - Marker outputs, 5 sec to 1 μ s. Sinewave available at 20, 10, and 2 ns. Trigger pulses 1, 10, 100 Hz; 1, 10, and 100 kHz. Multiple time-marks can be generated simultaneously.
181	TG 501 - Marker outputs, 5 sec to 1 ns. Sinewave available at 5, 2, and 1 ns.	181 - Marker outputs, 1, 10, 100, 1000, and 10,000 μ s, plus 10 ns sinewave.
184	TG 501 - Marker outputs, 5 sec to 1 ns. Sinewave available at 5, 2, and 1 ns. Trigger output - slaved to marker output from 5 sec through 100 ns. One time-mark can be generated at a time.	184 - Marker outputs, 5 sec to 2 ns. Sinewave available at 50, 20, 10, 5, and 2 ns. Separate trigger pulses of 1 and .1 sec; 10, 1, and .1 ms; 10 and 1 μ s. Marker amplifier provides positive or negative time marks of 25 V min. Marker intervals of 1 and .1 sec; 10, 1, and .1 ms; 10 and 1 μ s.
2901	TG 501 - Marker outputs, 5 sec to 1 ns. Sinewave available at 5, 2, and 1 ns. Trigger output - slaved to marker output from 5 sec through 100 ns. One time-mark can be generated at a time.	2901 - Marker outputs, 5 sec to 0.1 μ s. Sinewave available to 50, 10, and 5 ns. Separate trigger pulses, from 5 sec to 0.1 μ s. Multiple time-marks can be generated simultaneously.

NOTE: All TM 500 generator outputs are short-proof. All TM 500 plug-in instruments require TM 500-Series Power Module.



MANUAL CHANGE INFORMATION

PRODUCT DF 1
DISPLAY FORMATTER

CHANGE REFERENCE C2/677
DATE 6-7-77

CHANGE:

DESCRIPTION

070-2150-00

TEXT CORRECTIONS

SECTION 4 MAINTENANCE

Page 4-7 Keyboard Test

ADD: The following text after the last paragraph above TABLE 4-4:

The Keyboard Circuit Checkout Procedure (Table 4-4) checks the operation of a shift register. Therefore, the procedural steps must be performed in the exact sequence listed. An operator error incurred during the performance of this procedure invalidates the sequence, and step 1 of the Keyboard Circuit Checkout Procedure must be started again.

Page 4-7 TABLE 4-4, step 1 Comment column

ADD: No check; proceed to step 2.

Page 4-8 BUTTON LIGHTS TEST

ADD: The following NOTE after step b:

NOTE

All button lights that are on at the start of this test will be shifted to the right and down with each press of the Deposit button.

REMOVE: Step e.

Page 4-8 DISPLAY TEST

ADD: The following text to step a.

Assure that the System Test Fixture ABA indicator light is on. Turn off the oscilloscope power momentarily. This action will load WOM RAM with random data for future display. Disregard the actual data that is displayed in the following checks. It's only purpose is to provide a method to check the mode of operation.

CHANGE:	DESCRIPTION
Page 4-9 CHANGE TO READ:	TABLE 4-6, Display Column
Line #2	7D01 Timing diagram display with 2 lines of DF1 readout, if triggered. ¹
Line #3	Display 7D01 timing diagram only--no DF1 readout, if triggered. ¹
REMOVE:	Line #4
CHANGE:	Line #5 to Line #4
CHANGE:	Footnote ¹ to read:
	If the 7D01 is not triggered, check that 7D01 SAMPLE INTERVAL switch is not in the EXTERNAL position, and press the MANUAL TRIGGER button; verify performance of the 7D01. Check DF1's "7D01 reset" circuit.
Page 4-10	DISPLAY TEST
REMOVE:	Line "5" from step f.
Page 4-10	1. Cursor Increment.
ADD:	"See note below" to step b.
Page 4-11	1. CURSOR ACQUISITION
CHANGE:	Step a from 0-15 to 0-3.
ADD:	To step g "and remain on".