


**TDSHT3
HDMI Compliance Test Software
Quick Start User Manual**

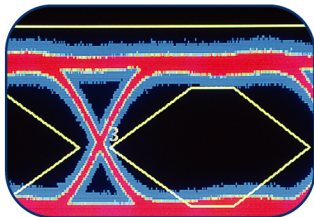


077-0119-00

Tektronix

**TDSHT3
HDMI Compliance Test Software
Quick Start User Manual**

This document applies to TDSHT3 version 3.3.0 and above, which supports HDMI CTS 1.3b1 specifications.

www.tektronix.com

077-0119-00

Tektronix

Copyright © Tektronix. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Contacting Tektronix

Tektronix, Inc.
14200 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
USA

For product information, sales, service, and technical support:

- In North America, call 1-800-833-9200.
- Worldwide, visit www.tektronix.com to find contacts in your area.

Warranty 9(b)

Tektronix warrants that the media on which this software product is furnished and the encoding of the programs on the media will be free from defects in materials and workmanship for a period of three (3) months from the date of shipment. If any such medium or encoding proves defective during the warranty period, Tektronix will provide a replacement in exchange for the defective medium. Except as to the media on which this software product is furnished, this software product is provided "as is" without warranty of any kind, either express or implied. Tektronix does not warrant that the functions contained in this software product will meet Customer's requirements or that the operation of the programs will be uninterrupted or error-free.

In order to obtain service under this warranty, Customer must notify Tektronix of the defect before the expiration of the warranty period. If Tektronix is unable to provide a replacement that is free from defects in materials and workmanship within a reasonable time thereafter, Customer may terminate the license for this software product and return this software product and any associated materials for credit or refund.

THIS WARRANTY IS GIVEN BY TEKTRONIX WITH RESPECT TO THE PRODUCT IN LIEU OF ANY OTHER WARRANTIES, EXPRESS OR IMPLIED. TEKTRONIX AND ITS VENDORS DISCLAIM ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. TEKTRONIX' RESPONSIBILITY TO REPLACE DEFECTIVE MEDIA OR REFUND CUSTOMER'S PAYMENT IS THE SOLE AND EXCLUSIVE REMEDY PROVIDED TO THE CUSTOMER FOR BREACH OF THIS WARRANTY. TEKTRONIX AND ITS VENDORS WILL NOT BE LIABLE FOR ANY INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES IRRESPECTIVE OF WHETHER TEKTRONIX OR THE VENDOR HAS ADVANCE NOTICE OF THE POSSIBILITY OF SUCH DAMAGES.

Table of Contents

General Safety Summary	iii
Preface	iv
Key Features	iv
Documentation	v
Software Upgrades	v
Install the Software	1
Before Installation	1
Installation	1
Connect to the Oscilloscope	2
Start the Software	3
Close the Software	6
Get Acquainted with the Software	7
Use the Interface	7
Set Preferences	10
Hide and Return the TDSHT3 Software	11
Use the TDSHT3 HDMI Software	13
Tests: Process Flow	13
Select a Test	13
Configure the Test Parameters	14
Connect and Configure the Equipment	14
View the Waveform	15
Run the Test	15
Interpret the Test Result	16
Generate and Print a Report	18
Application Examples	20
Source: Select All (Differential Tests)	20
Sink: Min/Max-Diff Swing Tolerance Test	22
Sink: Jitter Tolerance Test	24
Cable: Eye Diagram Test	29
Enable Remote Control of Test Equipment	32
Index	

General Safety Summary

Review the following safety precautions to avoid injury and prevent damage to this product or any products connected to it.

To avoid potential hazards, use this product only as specified.

Only qualified personnel should perform service procedures.

While using this product, you may need to access other parts of a larger system. Read the safety sections of the other component manuals for warnings and cautions related to operating the system.

To Avoid Fire or Personal Injury

Connect and Disconnect Properly. Connect the probe output to the measurement instrument before connecting the probe to the circuit under test. Connect the probe reference lead to the circuit under test before connecting the probe input. Disconnect the probe input and the probe reference lead from the circuit under test before disconnecting the probe from the measurement instrument.

Observe All Terminal Ratings. To avoid fire or shock hazard, observe all ratings and markings on the product. Consult the product manual for further ratings information before making connections to the product.

Do not apply a potential to any terminal, including the common terminal, that exceeds the maximum rating of that terminal.

Do Not Operate Without Covers. Do not operate this product with covers or panels removed.

Do Not Operate With Suspected Failures. If you suspect that there is damage to this product, have it inspected by qualified service personnel.

Avoid Exposed Circuitry. Do not touch exposed connections and components when power is present.

Do Not Operate in Wet/Damp Conditions.

Do Not Operate in an Explosive Atmosphere.

Keep Product Surfaces Clean and Dry.

Terms in this Manual

These terms may appear in this manual:



WARNING. Warning statements identify conditions or practices that could result in injury or loss of life.



CAUTION. Caution statements identify conditions or practices that could result in damage to this product or other property.

Preface

The TDSHT3 HDMI Compliance Test Software is a High Definition Multimedia Interface (HDMI) Compliance Test Solution, which runs on a Tektronix oscilloscope. This software helps you perform HDMI physical layer validation and compliance testing.

NOTE. You will be provided with two TDSHT3 applications, one supporting CTS 1.2a specification displayed as TDSHT3 and the other supporting CTS 1.3b1 specification displayed as TDSHT3v1.3. Both these applications can be loaded onto the oscilloscope but you can run only one application at a time. For more information on TDSHT3 supporting CTS1.2a specification refer to the TDSHT3 HDMI Quick Start User Manual (Tektronix part number: 071-1961-01).

Key Features

- Conformance to HDMI 1.3a standards and test specifications (CTS version 1.3b1) ensures reliable results
- Complete validation to standards with wide range of tests for source, sink, and cable devices
- Accurate source tests using precise measurement techniques
- Dependable sink tests with closed-loop measurements that eliminate nonlinearities in test setup
- Automated sink and cable tests with remote control of signal sources
- Automatic mask fit, measurements, and pass or fail notification
- In-depth analysis with statistical analysis and mask margins
- One-button selection of multiple tests
- One-button csv-format summary and HTML consolidated reports
- Complete compliance solution with an elaborate test fixture, signal sources, and TDR
- Source Single-Ended tests can be performed on two lanes
- Source Differential and Cable Eye diagram tests can be performed on all four lanes: Clock, Data0, Data1, and Data2

Documentation

This manual describes the installation and basic operation of the TSDHT3 software. For more detailed information, see the online help. The following information is available for this product:


TDSHT3 Online Help



Start > Programs > TekApplications > TDSHT3v1-3 > Help


TDSHT3 Online Help (PDF)

TDSHT3 Quick Start User Manual,
English (PDF)



TDSHT3 Quick Start User Manual,
Japanese (PDF)

TDSHT3 Quick Reference Card,
Source Test (PDF)




TDSHT3 Quick Reference Card,
Sink Test (PDF)

C:\ProgramFiles\TekApplications\TDSHT3v1-3\Manuals



www.tektronix.com/manuals

Installation Manual: *Optional*
Application Software on
Windows-Based Oscilloscopes



Software Upgrades

Periodic software upgrades may become available. Note that the software is only operational if you have a valid option key for the specific oscilloscope model and serial number.

To check for upgrades:

1. Go to www.tektronix.com/software.
2. Enter the product name (**TDSHT3**).

Install the Software

The TDSHT3 software must be installed on a Tektronix oscilloscope.

The 4-Channel feature allows you to perform Source/Cable tests on all four lanes (Clock, Data0, Data1, and Data2). The application generates a comprehensive test report for all channels when a measurement completes. It uses the real time capability of the DPO series oscilloscopes and reduces the testing time. It supports the following oscilloscopes:

- DPO70804 and DSA70804 (recommended)
- DPO71254 and DSA71254
- DPO71604 and DSA71604
- DPO72004 and DSA72004

This version of the TDSHT3 software also works on the following oscilloscopes but the 4-Channel feature is not supported:

- TDS7254 and TDS7254B
- TDS7404 and TDS7404B
- CSA7404 and CSA7404B
- TDS7704B
- TDS6604B
- TDS6804B
- TDS6124C
- TDS6154C
- DPO70404 and DSA70404
- DPO70604 and DSA70604

Before Installation

- TekVisa must be installed on the oscilloscope. If you do not have TekVisa, you can download it from the Tektronix Web site, in the same location as for *Software Upgrades*. (See page v, *Software Upgrades*.)
- Please read the Readme.txt file on the product software CD before you install the software.

Installation

1. Close all applications.
2. Insert the product software CD into the CD drive of the oscilloscope.
3. The installation wizard will guide you through the installation. If this is a version upgrade, the existing software will be automatically removed before the new version is installed.
4. The software files will be installed at C:\Program Files\TekApplications\TDSHT3v1-3.

Connect to the Oscilloscope

Each test requires specific equipment setups and specific test adapters. Click **More** within the connect pane to see how to connect the device under test and test equipment to your oscilloscope. The following test adapters are required, depending on the tests that you will be running:

- ET-HDMI-TPA-R, available from Efficere Technologies (recommended)
- ET-HDMI-TPA-P, available from Efficere Technologies (recommended)


The test fixtures mentioned below can only work for limited HDMI resolutions.

- Tektronix HDMI TPA-P-DI (for Differential Source tests except Eye Diagram)
- Tektronix HDMI TPA-P-SE (for Single-Ended Source tests)
- Tektronix HDMI TPA-P-TDR (for TDR tests) and Source tests (Eye Diagram)
- Tektronix HDMI TPA-R-DI (for Cable tests and Sink tests)
- Tektronix HDMI TPA-R-SE (for Cable tests and Sink tests)
- Tektronix HDMI TPA-R-TDR (for TDR tests and Sink tests)

Start the Software


To start the TDSHT3 software:

1. For TDS7000-series oscilloscopes, select **File > Run application > HDMI Compliance Test Software(1.3)**.

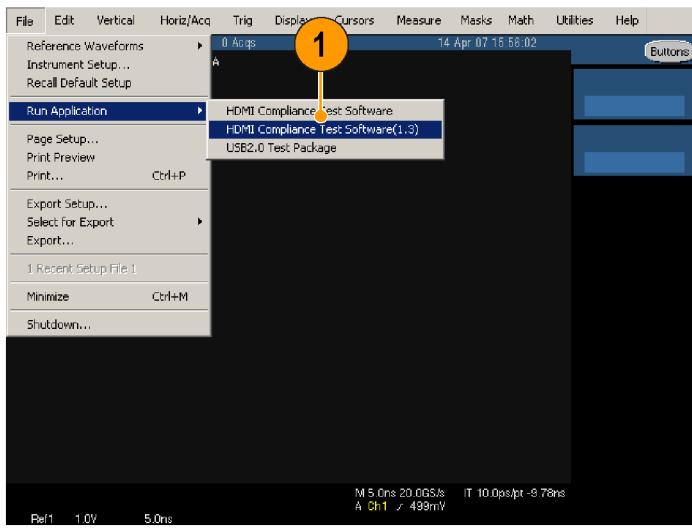


1981-003

2. For TDS B- and TDS C-series oscilloscopes, select **App > HDMI Compliance Test Software(1.3)**.

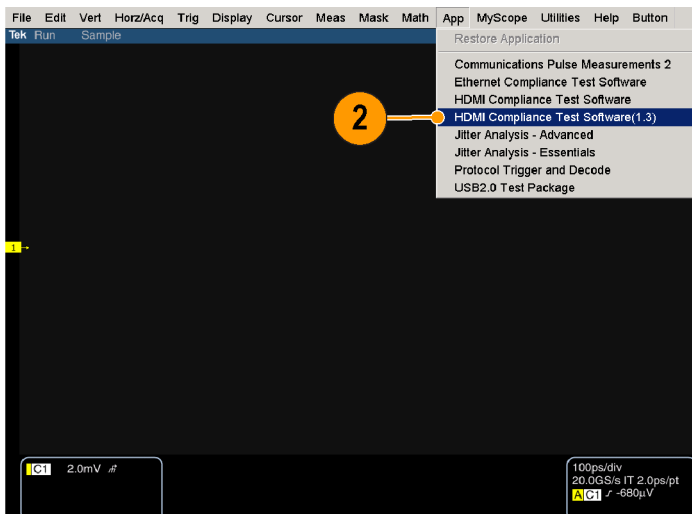


1981-004

- For DPO70000 and DSA70000-series oscilloscopes, select **Analyze > HDMI Compliance Test Software(1.3)**.

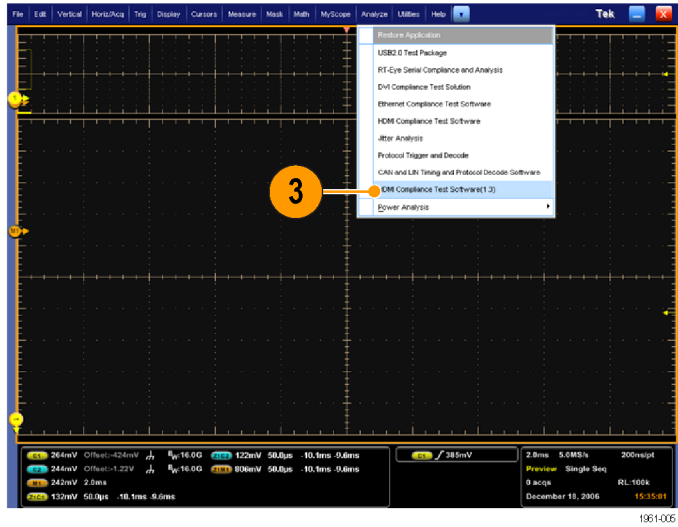

- The oscilloscope display resizes to fit in the upper part of the screen.
- The software displays in the lower part of the screen.

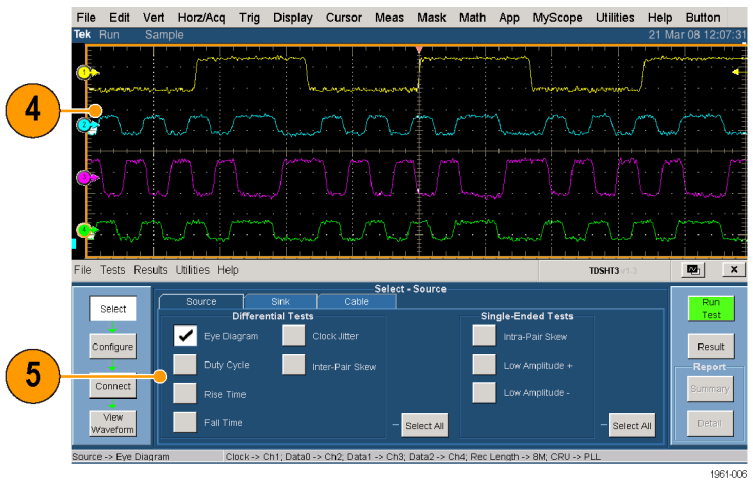


NOTE. To ensure accurate results, calibrate the probes and the oscilloscope before you run tests.

Calibrate the Probes and Oscilloscope


6. Click **Utilities > Instrument Calibration** to begin calibrating the oscilloscope for signal path compensation.
7. Click **Calibrate**.



8. Select **Vertical > Probe Cal** to begin calibrating the probes.
9. Connect the probe calibration signal to the probe.

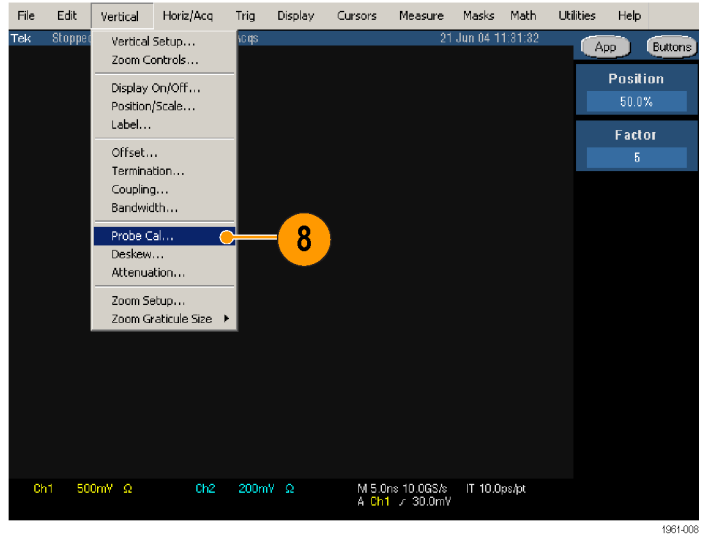


10. Click **Calibrate Probe**.

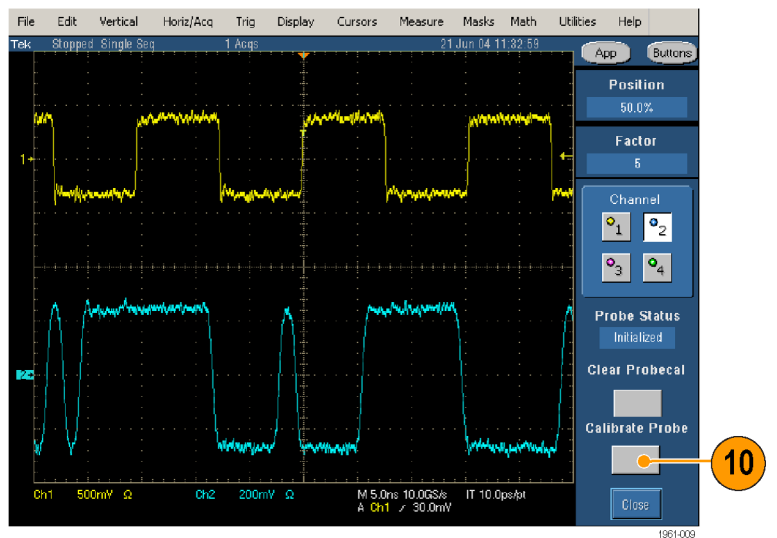

Close the Software

1. Select **File > Exit**.
2. You can also click the exit icon.
Using other methods to exit the software will result in abnormal termination.
3. When you exit the software, you can restore the oscilloscope to the settings that were in place before the TDSHT3 software changed them.

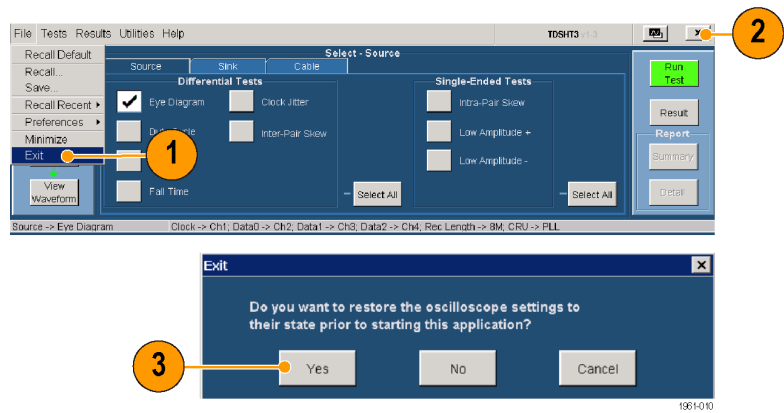


Get Acquainted with the Software

Use the Interface


Use a keyboard, mouse, or touch screen to make selections in the TDSHT3 software.

Use menus, check boxes, and on-screen buttons to control the software functions. Use Microsoft Windows techniques to navigate menus and select or clear check boxes.

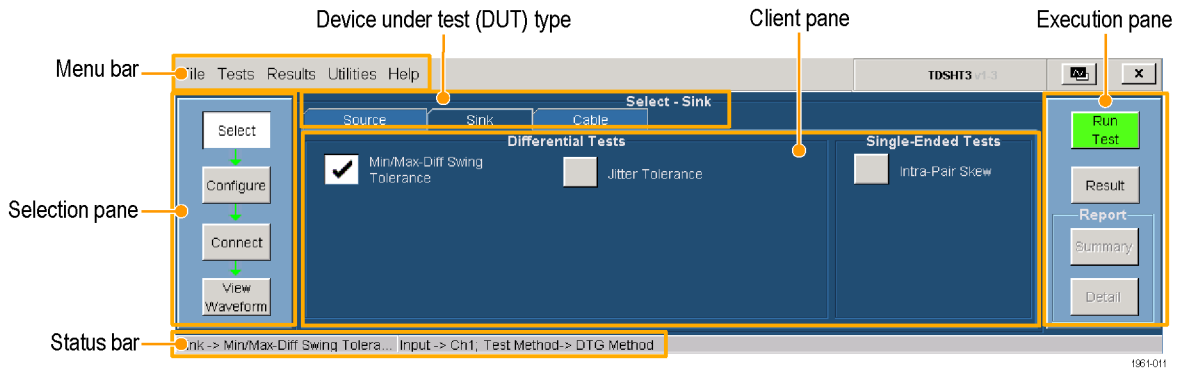

Virtual Keyboard

1. Click **New**.

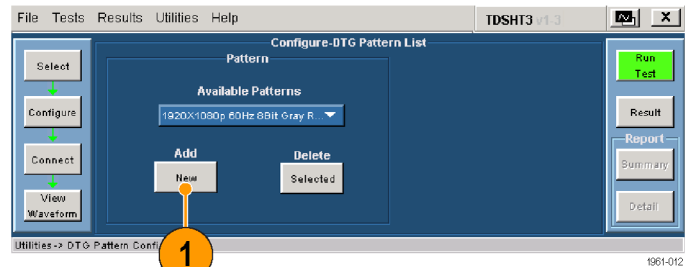


2. Clear the existing text and type the new text.
3. Click **Enter** to confirm your selection.




NOTE. You must click **Enter** on the virtual keyboard; otherwise your selections are not valid.

Virtual Keypad

1. Click any number box.
2. Click the keypad icon.

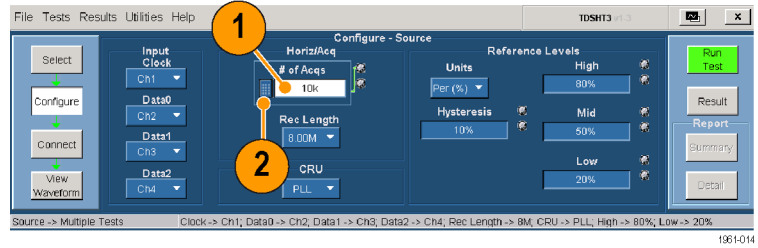


3. Clear existing value and enter the value desired.
4. Select a unit of measure.
5. Click **Enter** to confirm your selection.

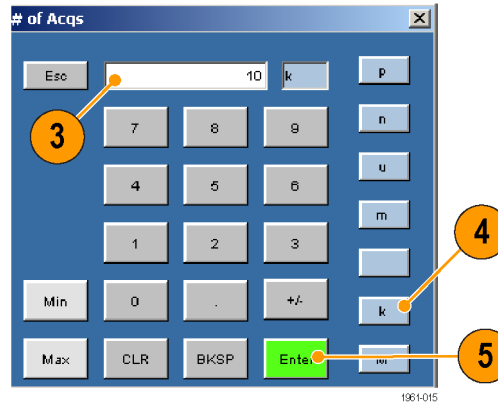


NOTE. You must click **Enter** on the virtual keypad; otherwise your selections are not valid.

General Purpose Knob

1. Click any number box to display the connection to one of the general purpose knobs.

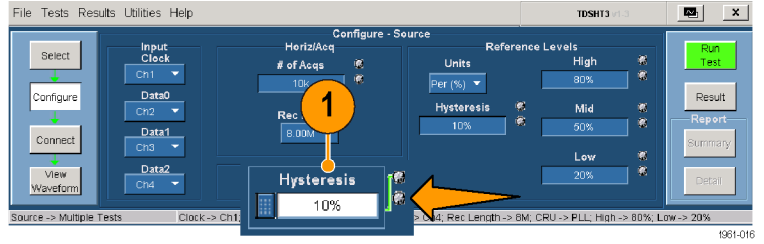


2. Turn the corresponding knob on the oscilloscope front panel to adjust the value for the selected parameter.
3. For better resolution, press the **FINE** button.

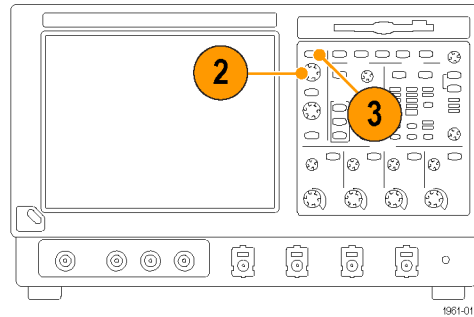

Set Preferences

1. From the TDSHT3 software menu bar, click **File > Preferences**, and then select an option.
2. Click the option again to clear the selection.

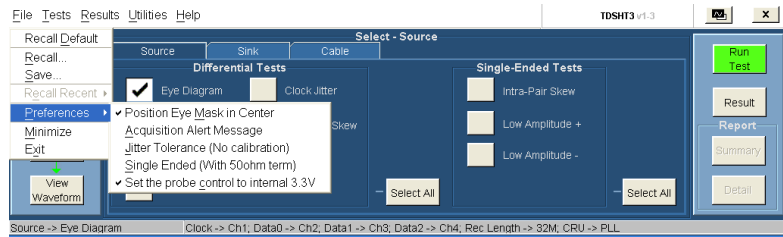


Option

Description

Position Eye Mask in Center	Selected: Positions the mask at the center of the eye diagram. Cleared: Positions the mask to the left of the eye diagram.
Acquisition Alert Message	Selected: An alert prompts you to specify oscilloscope settings with which to run the test. Cleared: TDSHT3 software selects oscilloscope settings.
Jitter Tolerance (No calibration)	Selected: Application will not run the jitter calibration test for Sink Jitter Tolerance measurements. Cleared: Application will run the jitter calibration test for Sink Jitter Tolerance measurements.
Single Ended (With 50 ohm term)	This option can be selected only when the negative input of the probe is terminated with the 50 ohm terminator. Selected: Application will run the single-ended measurements as though 50 ohm termination is connected. Cleared: Application will run the single-ended measurements without 50 ohm termination.
Set the probe control to internal 3.3V	This option is applicable to Source measurements on DPO/DSA oscilloscopes with P7313 probes. Selected: Application sets the probe control to internal and sets voltage to 3.3 V. Cleared: Application sets the probe control to Auto.


Hide and Return the TDSHT3 Software

1. Click the **hide** icon to minimize the TDSHT3 software and enlarge the oscilloscope display.

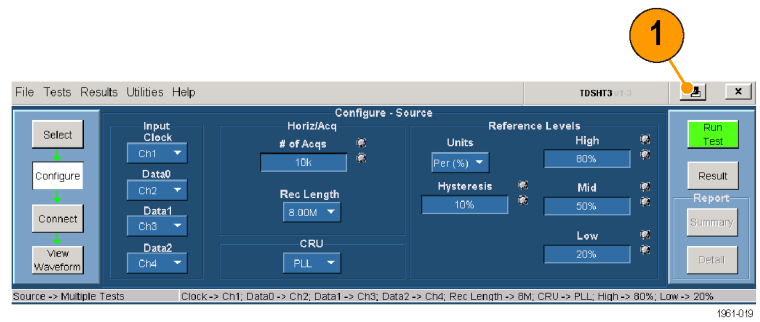


To return to the TDSHT3 software:


2. For TDS7000-series oscilloscopes, select the **APP** button.

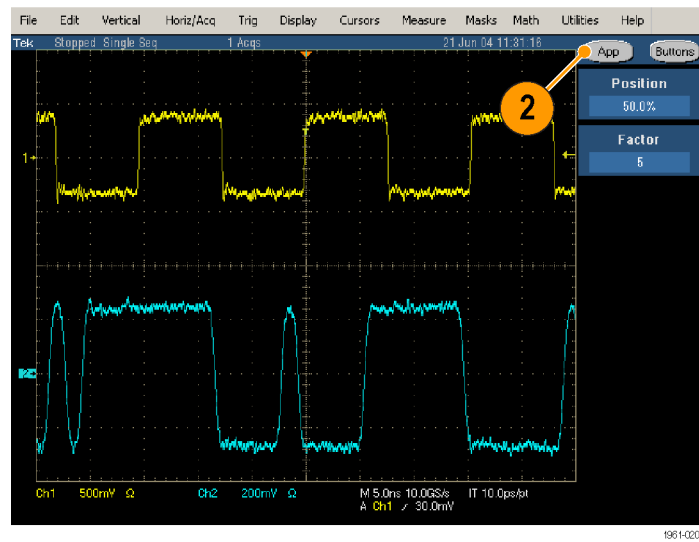

- For TDS6000B/C and TDS7000/B-series oscilloscopes, select **App > Restore Application**.

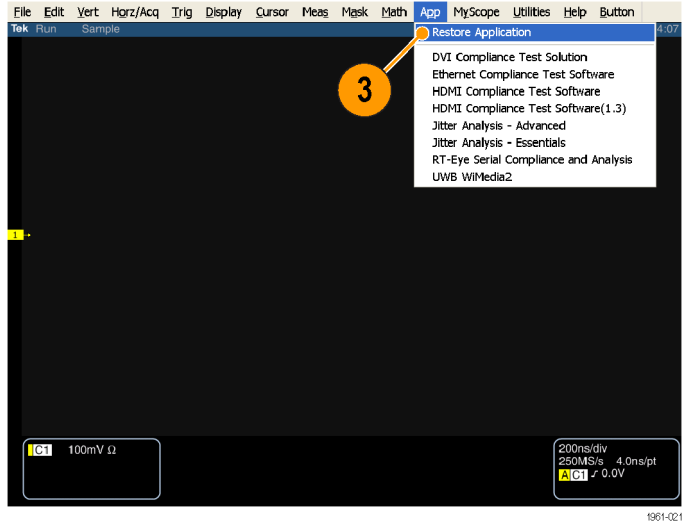

- For DPO70000 series oscilloscopes, select **Analyze > Restore Application**.

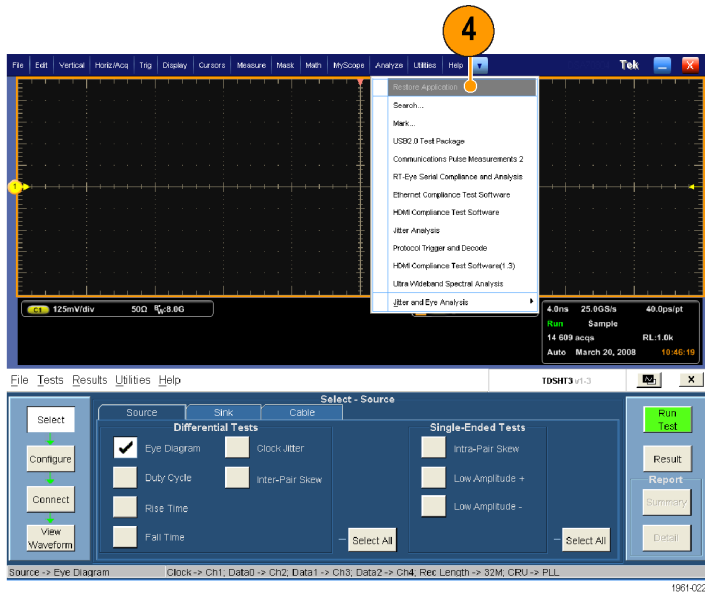


Use the TDSHT3 HDMI Software

Tests: Process Flow

When you make a test, follow the sequence of actions indicated in steps 1 through 6. Details for each of these actions are given on the following pages.


1. Select a test.
2. Configure the test parameters.
3. Connect and configure the equipment.
4. View the waveform to verify test signal.
5. Run the test.
6. Interpret the test result.
7. Generate a report.

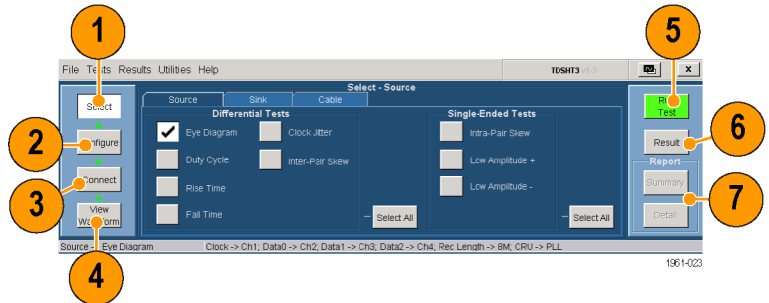

NOTE. For accurate test results, calibrate the oscilloscope and probes before you begin the tests. (See page 5, Calibrate the Probes and Oscilloscope.)


Select a Test

1. Click **Select**.
2. Click the **Source**, **Sink**, or **Cable** tab.
3. Move the mouse near a test name until the test ID appears. This ID corresponds to the Test ID in the HDMI Compliance Test Specifications.
4. Select the test that you want to run.
You can select multiple tests, but they must all be of the same type.
5. To select all tests of a certain type, click **Select All**.

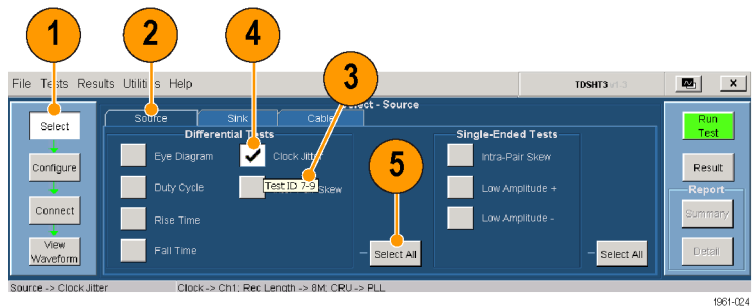

Configure the Test Parameters


1. Click **Configure**.
2. Use the virtual keyboard or the general purpose knob on the oscilloscope front panel to change the values if necessary. You can also use the File menu to restore factory defaults or save and recall your own configuration settings.

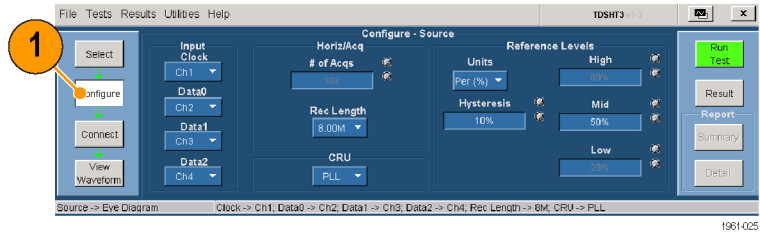

Connect and Configure the Equipment


NOTE. If your test uses remote control, the setup diagram in the online help shows how to connect the test equipment by using an E-net connection. You can either use this method or you can use the GPIB-B connection. (See page 32, *Enable Remote Control of Test Equipment.*) Example tests are shown in the *Application Examples* section. (See page 20.)

1. Click **Connect**.
2. Follow the on-screen instructions to connect and configure the device under test and the test equipment.
3. Click **More** to view the online help for the selected test, which contains a setup diagram. Connect the test equipment as shown in the diagram.
4. If the AWG/AFG and DTG are used for the selected test, select **Signal Sources** and configure the test equipment. (See page 32, *Enable Remote Control of Test Equipment.*)

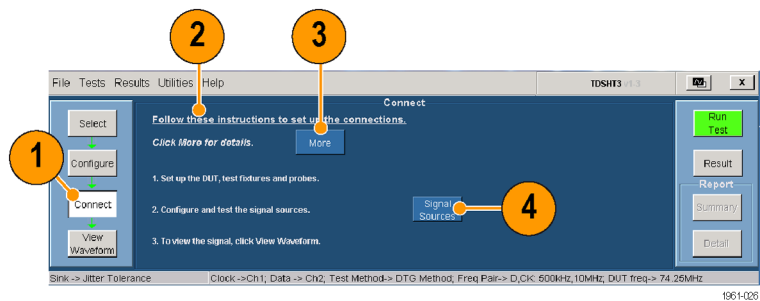

View the Waveform


1. Click **View Waveform** (not applicable for all tests).
2. Verify that the waveform in the upper part of display is similar to the waveform that is displayed in the TDSHT3 software.
If the displays are not similar, check your configuration and connections.

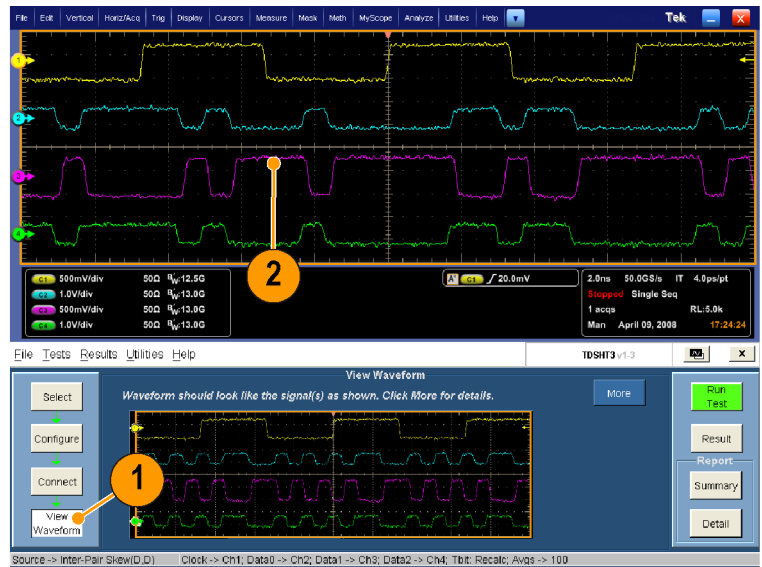

1961-027

Run the Test


1. Click **Run Test**.
2. The test will run, displaying a progress indicator.

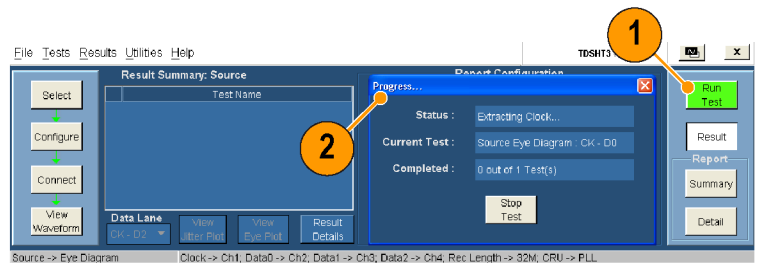



1961-028

Interpret the Test Result

1. When the test completes, the Result Summary appears. Check to see if the device passed the test.



 means Pass

 means Fail

 means Error

If the device did not pass the test, use steps 2 through 8 to solve the problem, and then rerun the test.

2. Click **Result Details** for a spreadsheet with details about the test result.
3. Check the Remarks column. If any error codes are present, see the online help for error code descriptions.

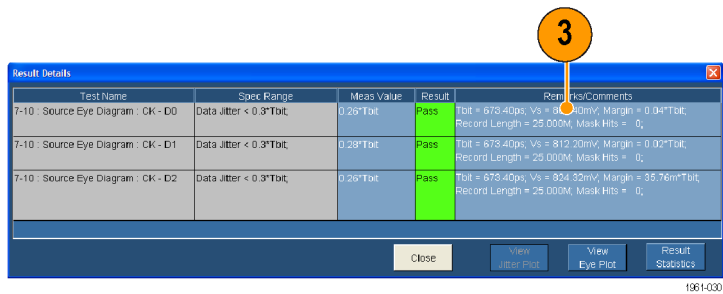
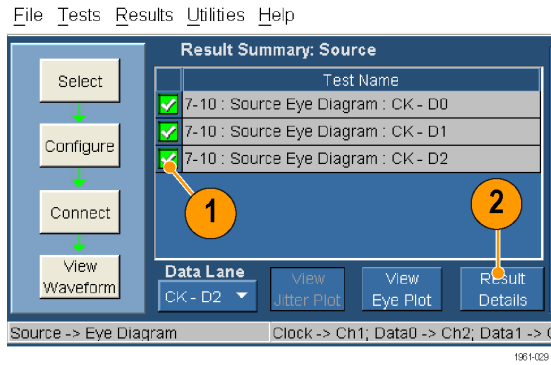


NOTE. The parameters in the Result Details dialog box may change depending on the test that you run.

The software displays the corresponding eye diagram depending on the option selected (CK-D0, CK-D1, or CK-D2) in the **Data Lane**. For example, CK-D0.

If you ran an eye diagram test, a plot appears. You can do the following:

4. Save the image to C:\TekApplications\TDSHT3v1-3\Images (you can also change this path).
5. Zoom in and out.
6. View the histogram.
7. Move the mask to see the margin of error.
8. View statistics.
9. Change the plot to half screen size (which returns the Result Summary).
10. A plot also appears if you ran the clock jitter test. In this plot, you will find the peak-to-peak jitter of the clock.

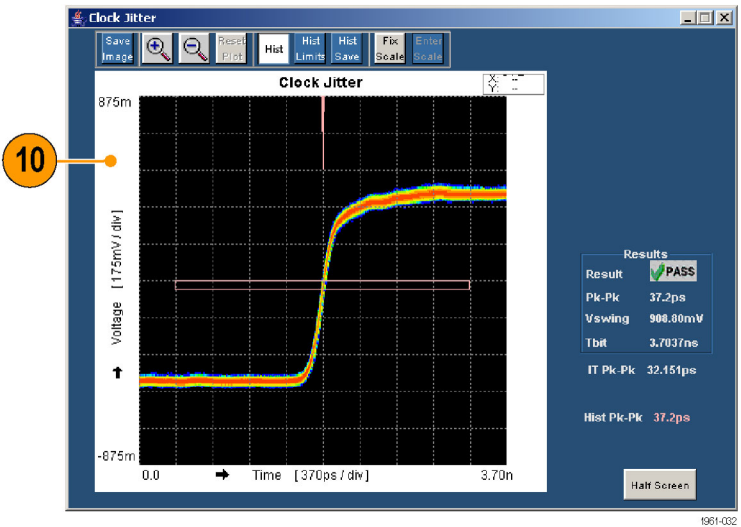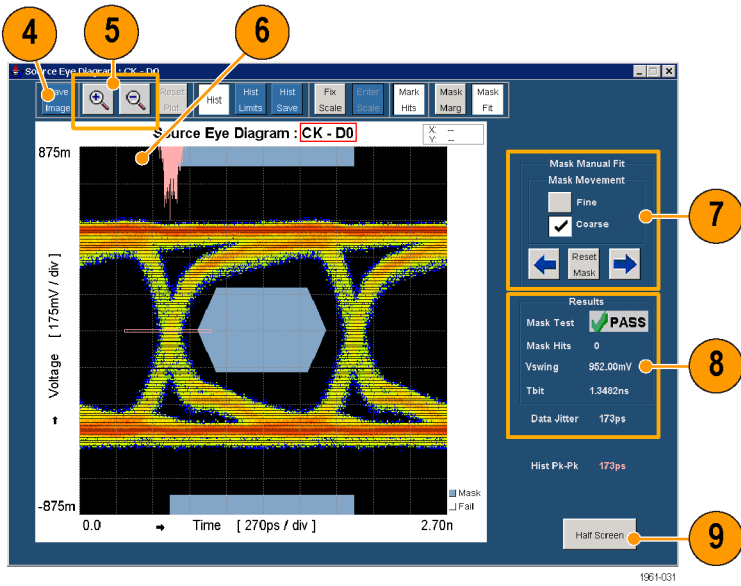


Generate and Print a Report

You can generate and print a summary or detailed report as described here.

Summary

After you have successfully run a test or tests, you can generate a report summary as a CSV file.


1. Click **Summary** in the execution pane.
2. A message indicates where the report summary is saved.
3. Open the file and print the report.

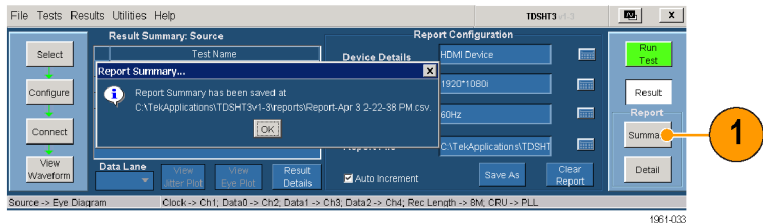



Detail

After you run a test, you can generate a report that contains default information or information that you configure.

1. Click **Result** to begin configuring the report (or skip to step 8 for defaults).
2. Enter the device details.
3. Enter the resolution at which you conducted the test (such as VGA, SVGA, XGA, SXGA, 1080i, or 1080p).
4. Enter the refresh rate at which you conducted the test (such as 50 Hz or 60 Hz).
5. Select **Auto Increment** to generate a new report. Selecting this option does not overwrite the existing report.
6. Click **Save As** to save the generated reports. The Save File dialog box is displayed. You can enter a file name and save the report.
7. Click **Clear Report** to clear all reports. Reports generated between this and the next successful test run will have no values.

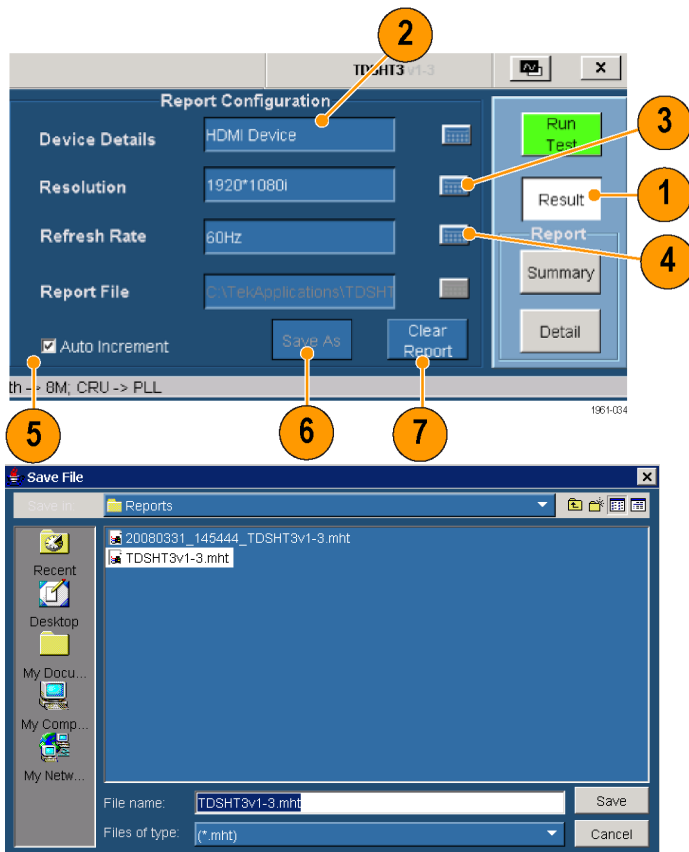

- 8. Click **Detail** in the report pane to generate the HTML report.
Plots and waveforms are displayed where ever applicable.

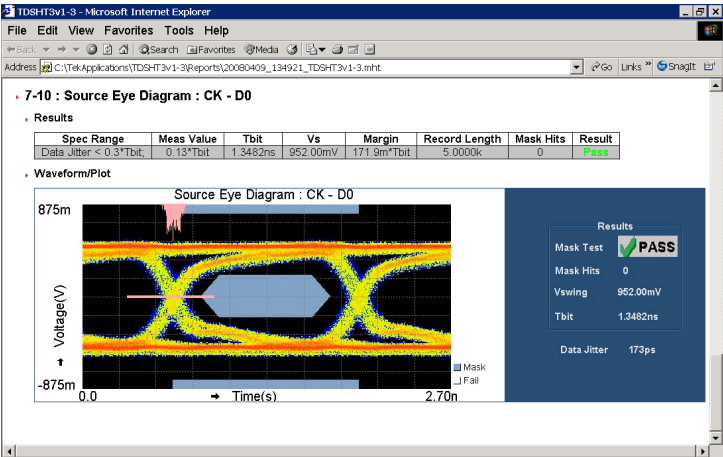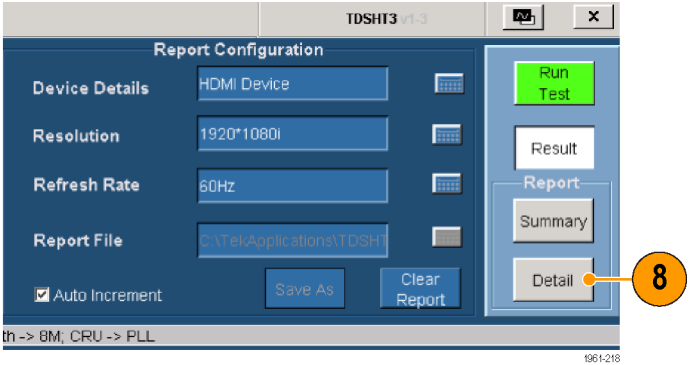

NOTE. The application generates an MHT file that can be opened in Internet Explorer.

Application Examples

Source: Select All (Differential Tests)

This selection runs a set of tests simultaneously.

Required equipment

2 (4 probes if you use four channels) differential probes; Ground lead

Example

Tektronix P7313SMA/P7350SMA (P7330/P7350/P7380/P7380SMA with external circuit can only be used with old fixtures);
 For P7313SMA probes with DPO/DSA, the internal bias voltage can be used in place of an external power supply.
 Tektronix part number 196-3469-00

1 DC power supply, set to 3.3 V

Kenwood PW18-1.8AQ

1 EDID emulator

ET-EDID PCB(INFO)/Silicon Image TE9100/Quantum Data 882CA


1 input adapter

ET-HDMI -TPA-P available from Efficere Technologies


Probe Calibration and Deskew fixture


Tektronix part number 067-1478-XX

1. Click **Select**.
2. Click the **Source** tab.
3. Click Select All.

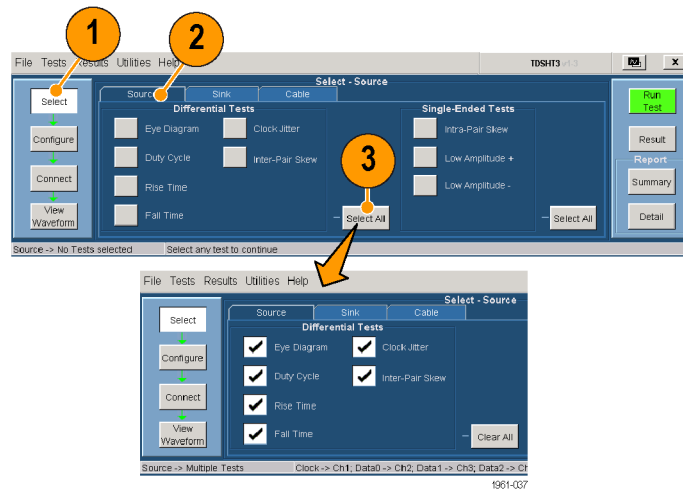


4. Click **Configure**. Change these values if needed. (You can generally use the default values.)

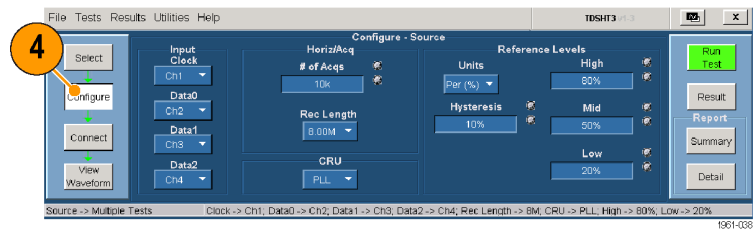

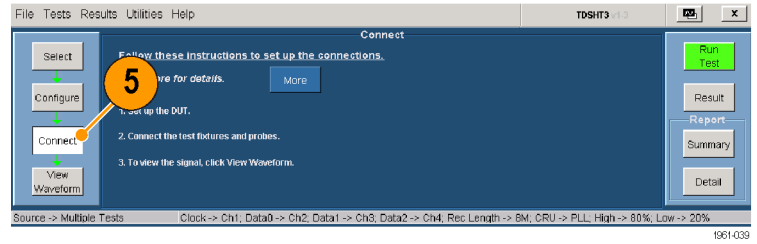5. Click **Connect**.

6. Connect and configure the equipment:


- Connect the test equipment as shown in the setup diagram.
- Configure the source DUT to output the first supported video format.
- Connect the Efficere EDID PCB with the EDID chip or configure the EDID Emulator for the required resolution (refer to the EDID Emulator user manual).

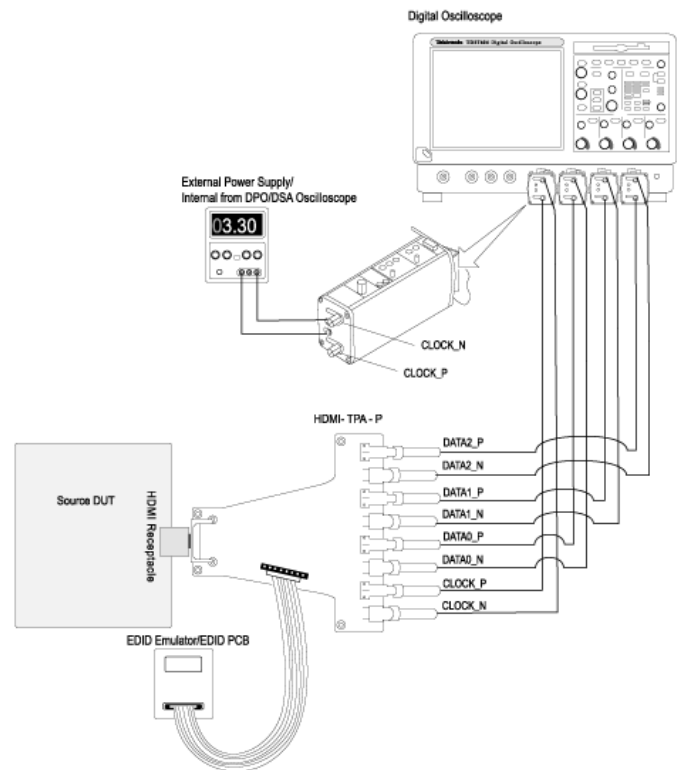

7. Click **View Waveform**.

Verify that the oscilloscope displays a similar waveform to the one displayed by the TDSHT3 software. If the displays are not similar, check your configuration and connections.


To ensure accurate results, deskew the probes before you run a test.

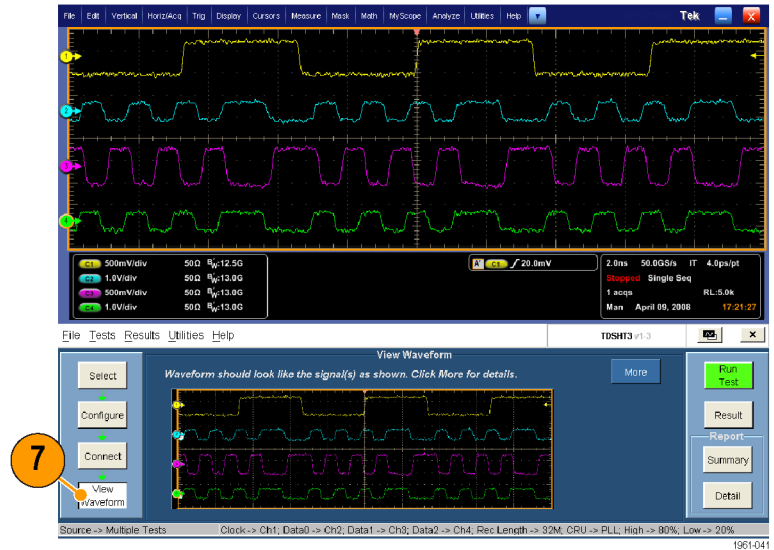

8. Click **Run Test**.

9. When the test completes, check the test results. (See page 16, *Interpret the Test Result*.)

10. You can generate reports based on the tests that you ran. (See page 18, *Generate and Print a Report*.)

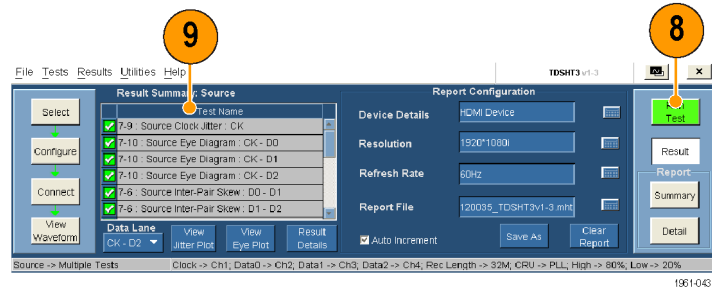

Sink: Min/Max-Diff Swing Tolerance Test

This test verifies that the sink device properly supports TMDS differential voltages at minimum levels.

Required equipment

Example

Digital Timing Generator

Tektronix DTG5274 (up to 2.7 Gb)/DTG5334 (up to 3.4 Gb) with DTGM30 output module

8 SMA cables

Tektronix part number 174-1341-00, 1 meter, or Tektronix part number 174-1428-00, 1.5 meters


1 DC power supply, set to 5.0 V

Kenwood PW18-1.8AQ



1 input adapter

ET-HDMI -TPA-P available from Efficere Technologies


1. Click **Select**.
2. Click the **Sink** tab.
3. Select **Min/Max-Diff Swing Tolerance**.

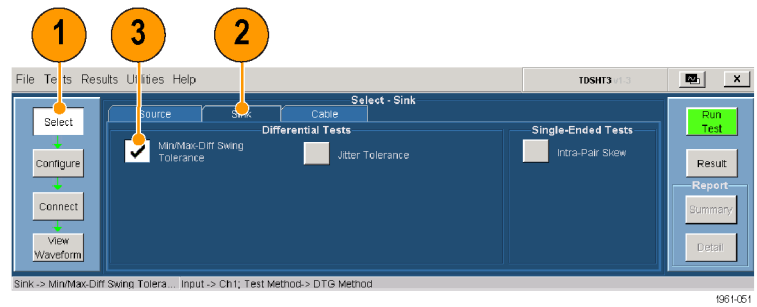

4. Click **Configure**. Change these values if needed. (You can generally use the default values.)
5. Select the pattern from the available options and click **Outputs** to configure the DTG Outputs.

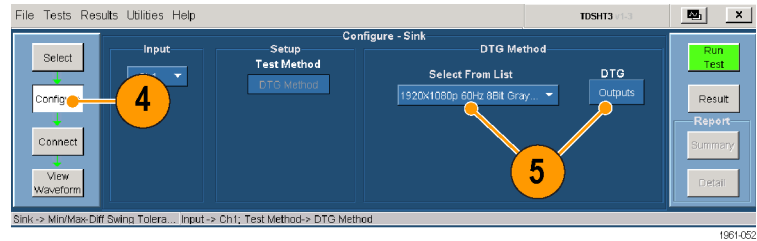


6. Click **Connect**.

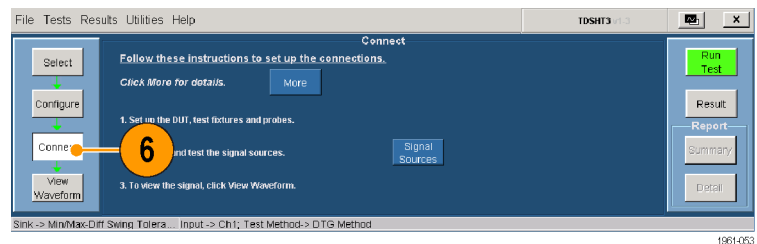

7. Connect and configure the equipment:

- Connect the test equipment as shown in the diagram.
- Connect the DTG and oscilloscope. (See page 32, *Enable Remote Control of Test Equipment.*)

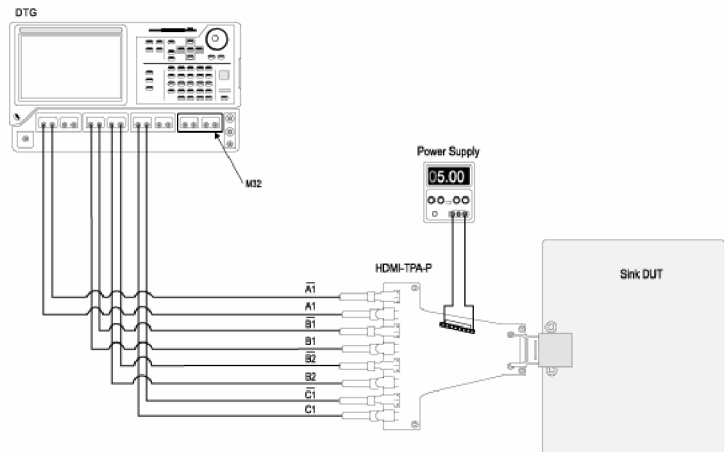


8. Click **Run Test**.

9. Follow the series of on-screen messages.

10. When the test completes, check the test results. (See page 16, *Interpret the Test Result.*)

11. You can generate reports based on the tests that you ran. (See page 18, *Generate and Print a Report.*)

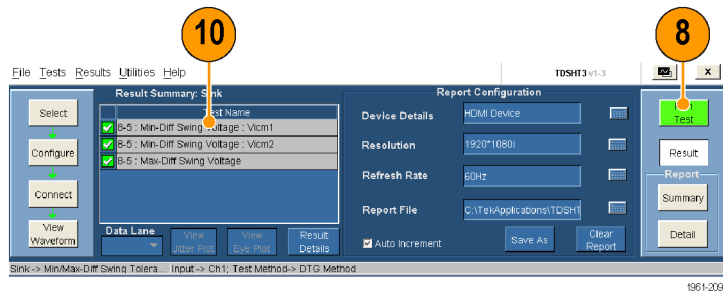

NOTE. When you run sink or cable tests, a warning about GPIB Bus Timing appears. If you are sure that the bus timing parameter is set to 2 μ sec, click OK to continue. Otherwise, click Cancel and change the bus timing parameter. (See page 37, *Set the GPIB Bus Timing.*)

Sink: Jitter Tolerance Test

This test verifies that your device supports the maximum allowed TMDS clock jitter.

Required equipment

Example

Digital Timing Generator	Tektronix DTG5274 (up to 2.7 Gb)/DTG5334 (up to 3.4 Gb) with DTGM30 and DTGM32 (for use with AWG710/AWG710B/AFG3000 only) output module
Arbitrary Waveform Generator	Tektronix AWG710 or AWG710B or AWG7102 (Separate Jitter insertion)
Arbitrary Function Generator	Tektronix AFG3102, AFG3022, AFG3252
12 SMA cables	Tektronix part number 174-1341-00, 1 meter, or Tektronix part number 174-1428-00, 1.5 meters
1 cable emulator	As described in CTS 1.3b1
2 bias tees	Mini-circuits ZFBT-4R2GW


Required equipment

- 1 DC power supply, set to 5 V
- 2 input adapters



Example

Kenwood PW18-1.8AQ
 ET-HDMI -TPA-P and ET-HDMI -TPA-R available from Efficere Technologies


1. Click **Select**.
2. Click the **Sink** tab.
3. Select **Jitter Tolerance**.

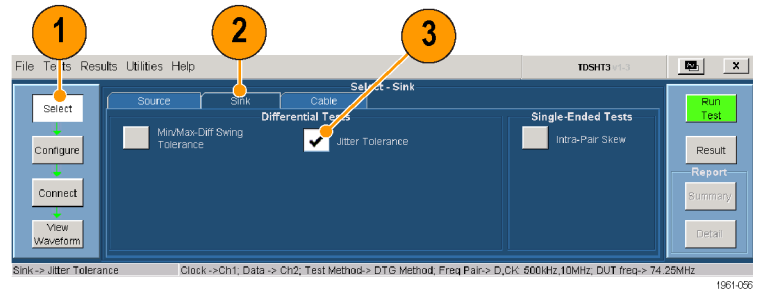

4. Click **Configure**. Change these values if needed. (You can generally use the default values.)
5. Select the pattern and jitter insertion type from the available options, and then click **Outputs** to configure the DTG Outputs.

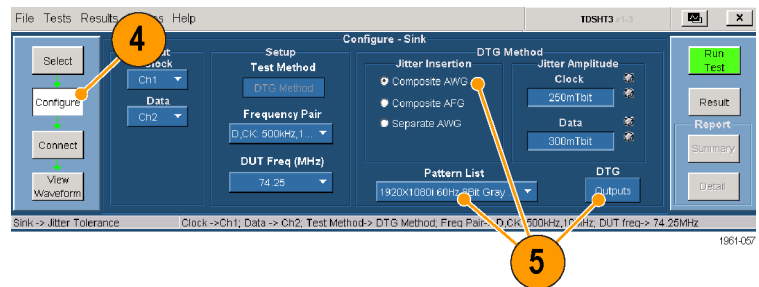


6. Click **Connect**.

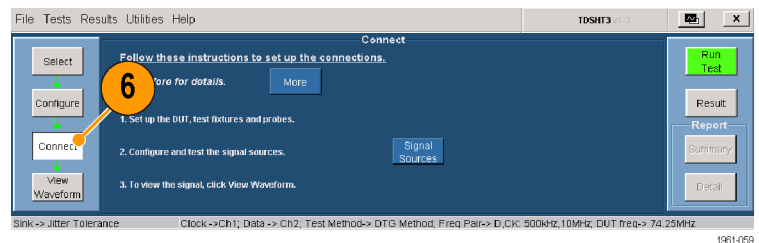


Method 1b: DTG-AWG710/AWG710B for testing resolutions >74.25 MHz

- Connect the test equipment to the DTG and AWG as shown in the setup diagram.
- When connecting the test fixture to the DUT, use a cable emulator specified for the pixel clock rate being tested.
- Connect the DTG, AWG, and oscilloscope according to the Enable Remote Control of Test Equipment procedure. (See page 32.)
- Configure the DUT to receive the HDMI input signal.

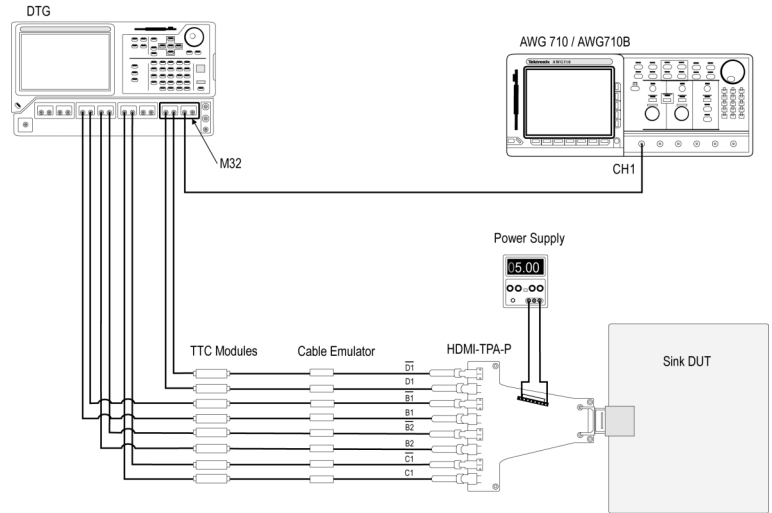


Method 2: DTG-AFG3000 composite jitter insertion

- Connect the test equipment to the DTG and AFG as shown in the setup diagram.
- When connecting the test fixture to the DUT, use a cable emulator specified for the pixel clock rate being tested.
- Connect the DTG, AFG, and oscilloscope according to the Enable Remote Control of Test Equipment procedure. (See page 32.)
- Configure the DUT to receive the HDMI input signal.

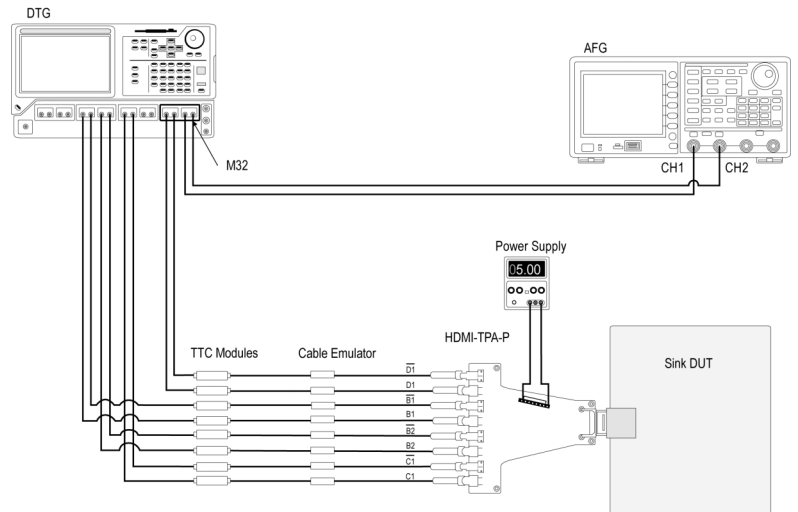


Method 3: DTG-AWG7102 composite jitter insertion for all frequencies

- Connect the test equipment to the DTG and AWG7102 as shown in the setup diagram.
- When connecting the test fixture to the DUT, use a cable emulator specified for the pixel clock rate being tested.
- Connect the DTG, AWG7102, and oscilloscope according to the Enable Remote Control of Test Equipment procedure. (See page 32.)
- Configure the DUT to receive the HDMI input signal.

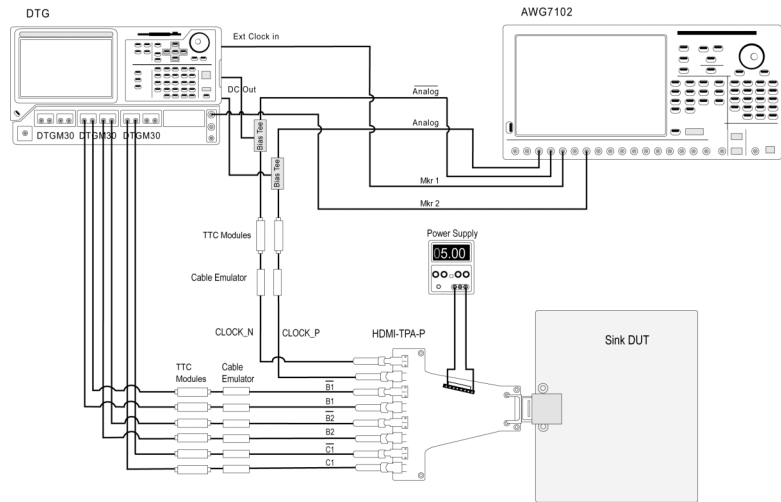


Method 4: DTG-AWG7102 separate jitter insertion for all frequencies

- Connect the test equipment to the DTG and AWG7102 as shown in the setup diagram.
- When connecting the test fixture to the DUT, use a cable emulator specified for the pixel clock rate being tested.
- Connect the DTG, AWG7102, and oscilloscope according to the Enable Remote Control of Test Equipment procedure. (See page 32.)
- Configure the DUT to receive the HDMI input signal.

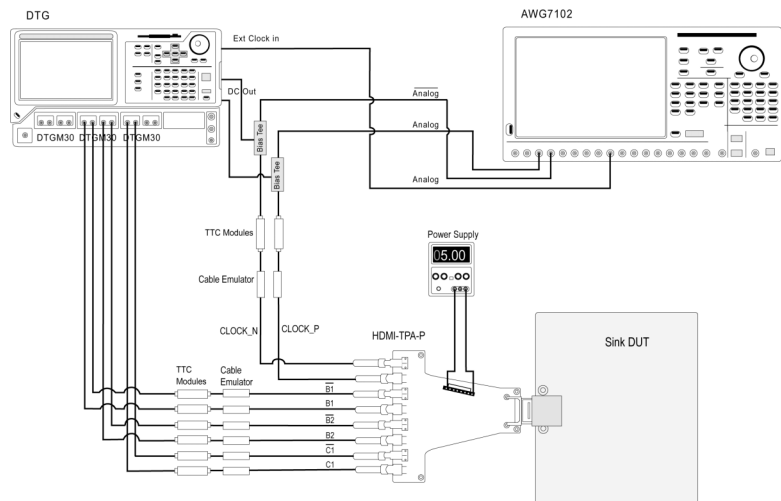

9. Click **Run Test**.
10. Follow the series of on-screen messages.
11. When the test completes, check the test results. (See page 16, *Interpret the Test Result*.)
12. You can generate reports based on the tests that you ran. (See page 18, *Generate and Print a Report*.)

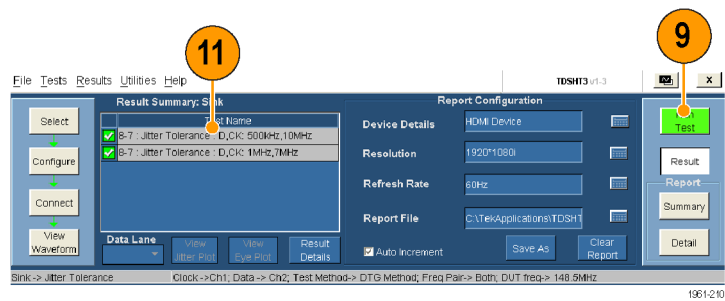

NOTE. When you run sink or cable tests, a warning about GPIB Bus Timing appears. If you are sure that the bus timing parameter is set to 2 μ sec, click OK to continue. Otherwise, click Cancel and change the bus timing parameter. (See page 37, Set the GPIB Bus Timing.)

Cable: Eye Diagram Test


Cable Equalizer

The signal degradation of typical passive copper cables increases with the frequency and the length of the cable. To recover data from such cables, the TDSHT3 applies the reference cable equalizer as specified in the HDMI specification 1.3 to Eye Diagram measurement when the clock frequency is more than 165 MHz.

This test verifies that the cable assembly outputs a compliant data eye.


Required equipment	Example
Digital Timing Generator	Tektronix DTG5274 (up to 2.7 Gb)/DTG5334 (up to 3.4 Gb) with three DTGM30 and DTGM32 (for use with AFG3000 only) output module
2 differential probes; Ground lead	Tektronix P7313SMA; Tektronix part number 196-3469-00
Arbitrary Function Generator	Tektronix AFG3102, AFG3022, AFG3252
8 SMA cables	Tektronix part number 174-1341-00, 1 meter, or Tektronix part number 174-1428-00 1.5 meters
1 DC power supply, set to 3.3 V	Kenwood PW18-1.8AQ
2 input adapters	ET-HDMI -TPA-P and ET-HDMI -TPA-R available from Efficere Technologies

1. Click **Select**.
2. Click the **Cable** tab.

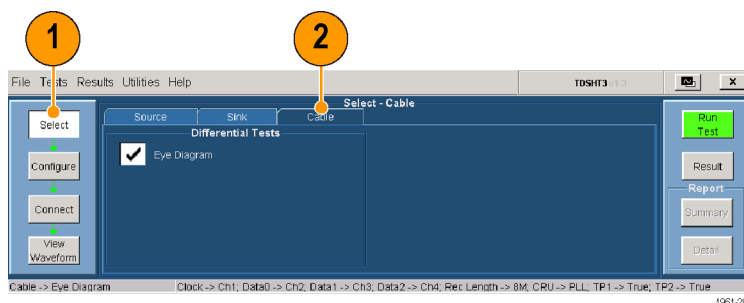


3. Click **Configure**. Change the values if needed. (You can generally use the default values.)

- **Test Points.** For the first cable that you test, select TP1 and TP2 to verify both the input test signal (TP1) and the output of the cable (TP2). For successive cable tests, clear TP1.
- **CRU.** Ensure that PLL (default) is selected for compliance testing.

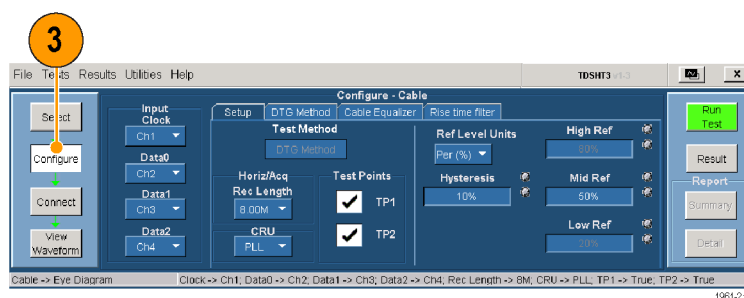


4. Click the **DTG Method** tab.


- Select the pattern and jitter insertion type from the available options.
- Configure the DTG outputs that will provide the clock and data input signals.

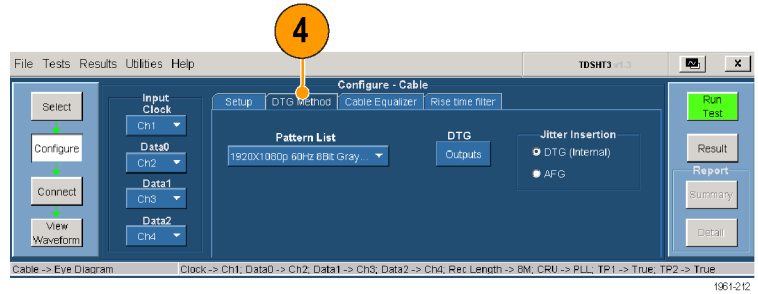

5. Click the **Cable Equalizer** tab to select the configuration options.

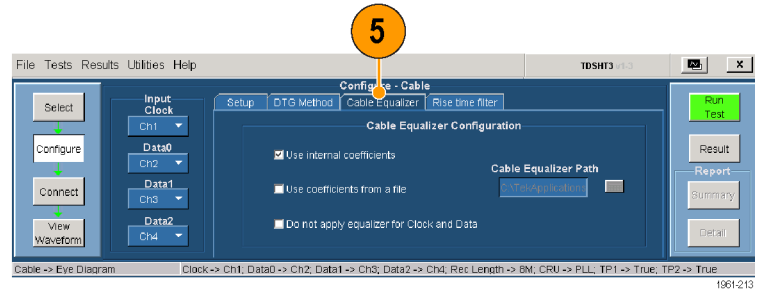

6. Click the **Rise Time Filter** tab to select the configuration options.

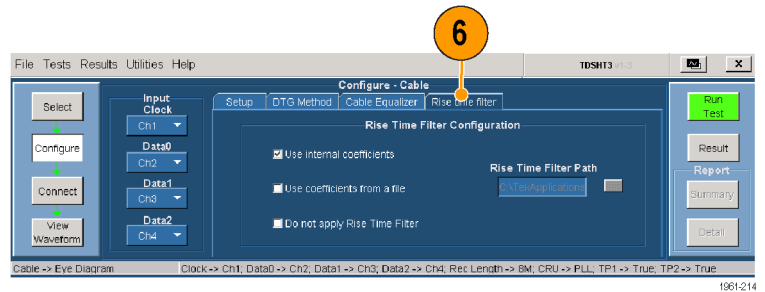


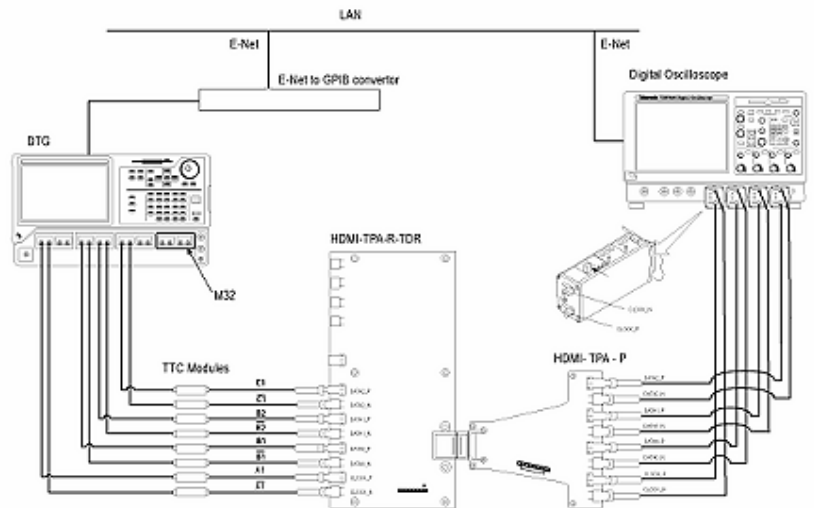
7. Click **Connect**.



8. Connect and configure the equipment to verify the test signal input:

- Connect the test equipment as shown in the TP1 setup diagram.
- Connect the DTG and oscilloscope. (See page 32, *Enable Remote Control of Test Equipment.*)

NOTE. In the diagram, the  symbol represents a 50 Ω termination or an unused probe input.




NOTE. When you run sink or cable tests, a warning about GPIB Bus Timing appears. If you are sure that the bus timing parameter is set to 2 μ sec, click OK to continue. Otherwise, click Cancel and change the bus timing parameter. (See page 37, *Set the GPIB Bus Timing.*)

9. Click **Run Test**.

10. Follow the series of on-screen messages.

11. When the test completes, check the test results. These results confirm that the test signal input is compliant. (See page 16, *Interpret the Test Result*.)

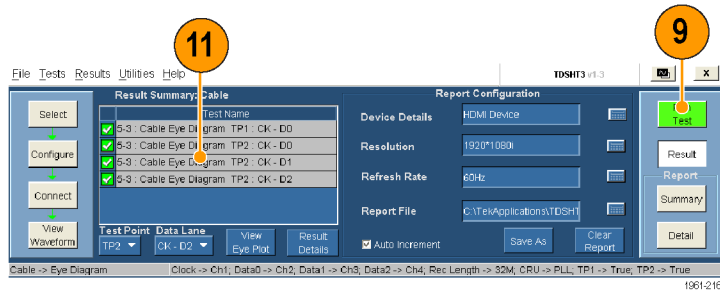


12. Remove the TPA-P-DI adapter and add the TPA-R-DI adapter as shown in the diagram.

NOTE. In the diagram, the **TERM** symbol represents a 50 Ω termination or an unused probe input.

13. Add the cable DUT between the TPA-R-TDR adapters.

14. Click **Run Test**.

15. When the test completes, check the test results. Pass indicates HDMI compliance of the cable DUT. (See page 16, *Interpret the Test Result*.)

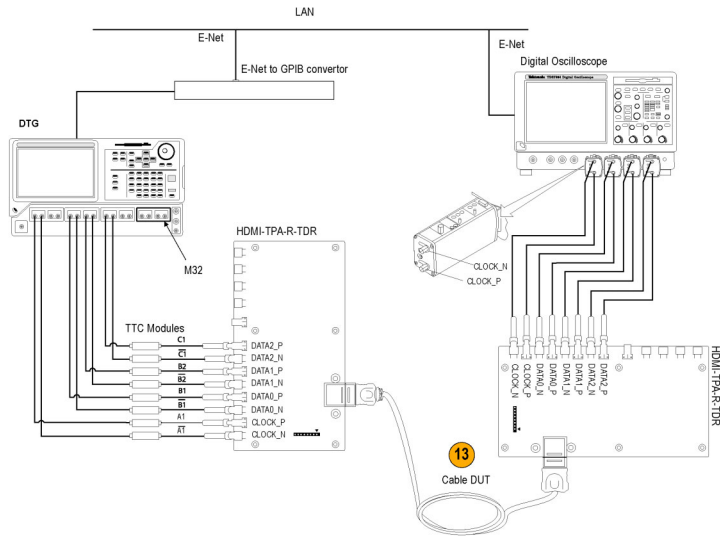

16. Click **Configure** and set the test point to TP2.

17. Replace the cable with another cable DUT and click **Run Test**.

18. You can generate reports based on the tests that you ran. (See page 18, *Generate and Print a Report*.)

Enable Remote Control of Test Equipment

If you are using the specified Tektronix DTG and AWG models, the TDSHT3 software can configure the connected test equipment automatically as you run tests. If you are using another DTG or AWG, you must configure the test equipment manually.

Use this procedure to:

- Connect the AWG and DTG for remote control
- Configure the GPIB address for remote control

You will need:

- Tektronix DTG5274 or DTG5334 and Tektronix AWG710 or AWG710B or AFG3000 (two channel model) or AWG7102
- Tektronix TDS7000 series oscilloscope, DPO70000 series digital oscilloscope, or DSA70000 series digital oscilloscope
- National Instruments GPIB-USB-B with the included software, NI-488.2 for Windows


NI-488.2 Software configuration for TDS series

NOTE. If you already have NI-488.2 installed on your oscilloscope, ensure that you have the version and installation parameters that are described in step 1. If you do not, then uninstall NI-488.2, and install it according to step 1.

1. Install NI-488.2 for Windows (version 2.1 or later).

During installation:

2. Do not install NI-VISA.
3. Install the Measurement & Automation Explorer.
4. When prompted, enable the GPIB-USB interface.
5. Restart the oscilloscope.

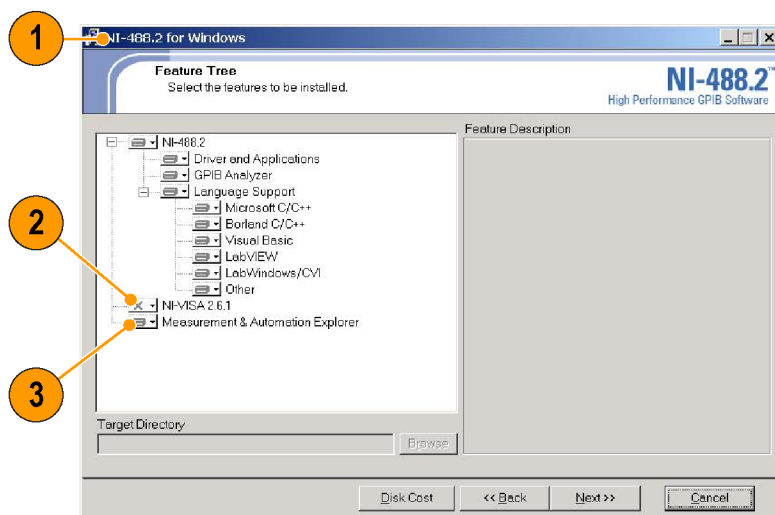


1961-076

NI-Software configuration for DPO70000/DSA70000 series

NOTE. If you are using the NI-Drivers on the DPO70000/DSA70000 series for the first time, perform steps 6 through 14. If not, perform steps 12 through 14.

- In the oscilloscope menu, click **Utilities > GPIB Configuration**.

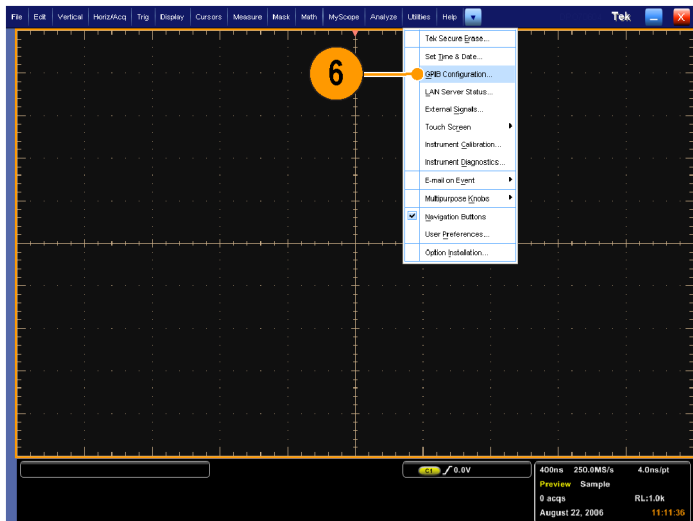

1961-078


- In the GPIB configuration, select **Controller**. A GPIB Mode Switch dialog box is displayed.

- Press **OK** to restart the oscilloscope.



1961-078

9. In the oscilloscope menu, click **Utilities > GPIB Configuration**.
10. In the GPIB configuration, select **Talk/Listen**. A GPIB mode switch dialog box is displayed.
11. Press **OK** to restart the oscilloscope.

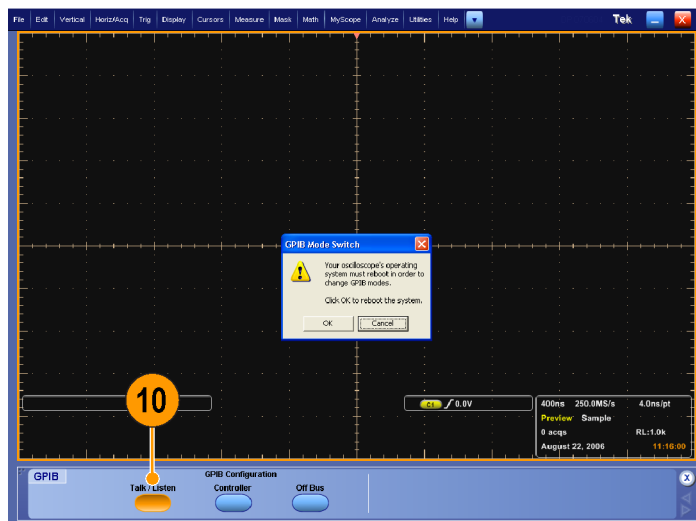

1961-079

You cannot access the NI software from the Start > Program menu. Instead, go to C:\Program Files\National Instruments\NI-488.2\Bin location.

12. Double-click on the Add GPIB Hardware to display the Add GPIB Hardware Wizard.
13. Select the appropriate NI hardware from the list (select GPIB-USB-B from the list if it is connected).
14. Press Next and finish the installation.




1961-080

NOTE. Do not install any NI drivers on the DPO70000 or DSA70000 series oscilloscope because they are preinstalled.


Connect the Equipment

15. Connect the USB-GPIB controller to the oscilloscope USB port. The oscilloscope operating system detects the USB-GPIB controller and installs the driver for it.
16. Using GPIB cables, connect (stack) the DTG and AWG/AFG GPIB connectors to the GPIB port of the GPIB controller. If your test does not use the AWG/AFG, connect the GPIB-USB-B between the oscilloscope and the DTG, omitting the stacked connector from the AWG/AFG.

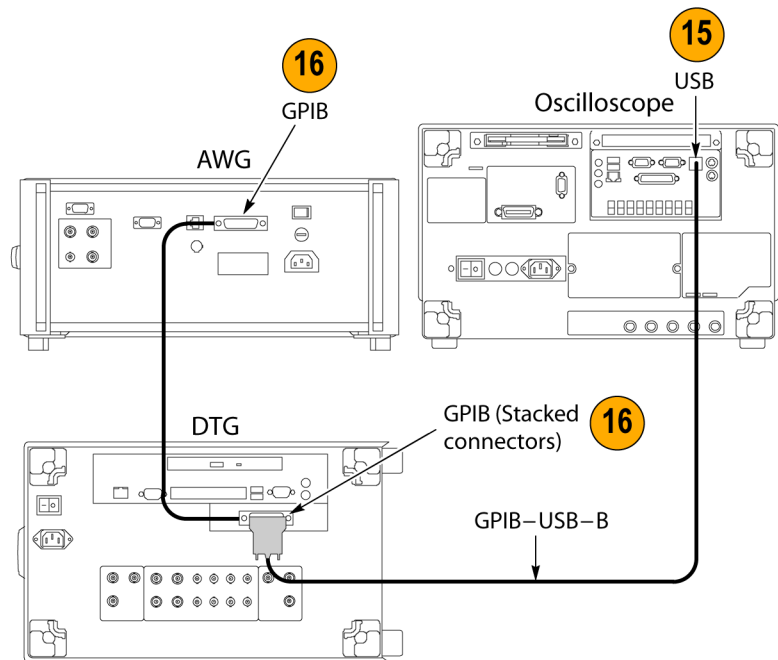


Verify the Equipment Connections

17. Open the Measurement & Automation Explorer that was installed with the NI-488.2 software.
18. In the Configuration pane, under Devices and Interfaces, right-click the GPIB device.
19. Click **Scan for Instruments**.
20. Note the GPIB Instrument Number and the Primary Address.
21. Right-click the instrument and click **Communicate with Instrument**.
22. Click **Query** and check that *IDN? describes the correct equipment.

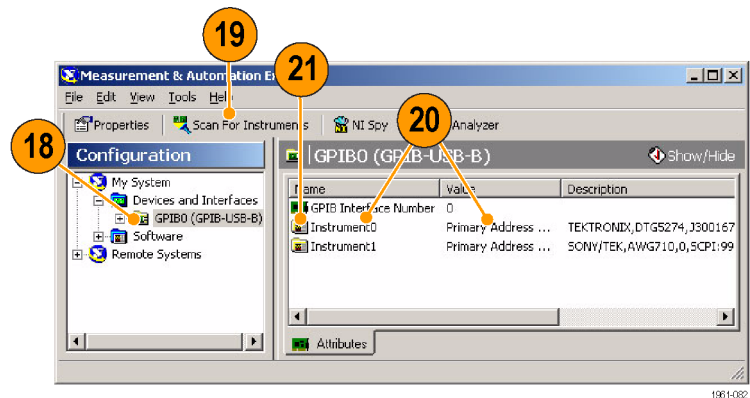


Set the GPIB Bus Timing

23. Right-click the GPIB device and click **Properties**.

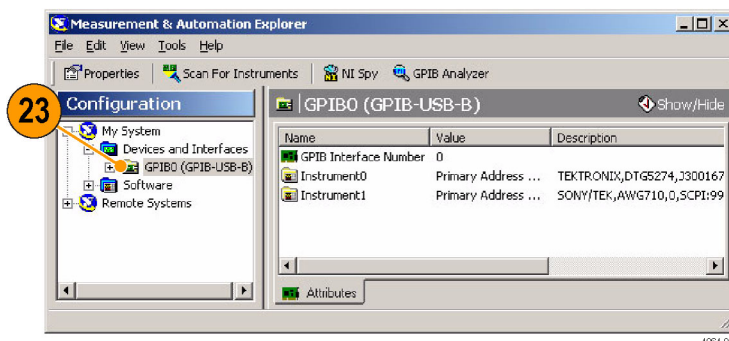

24. Click the **Advanced** tab.
25. In the Bus Timing list, select 2 μ sec.
26. Click **OK**. (Be sure that you complete the procedure through step 38, where you will exit the software and restart the oscilloscope.)

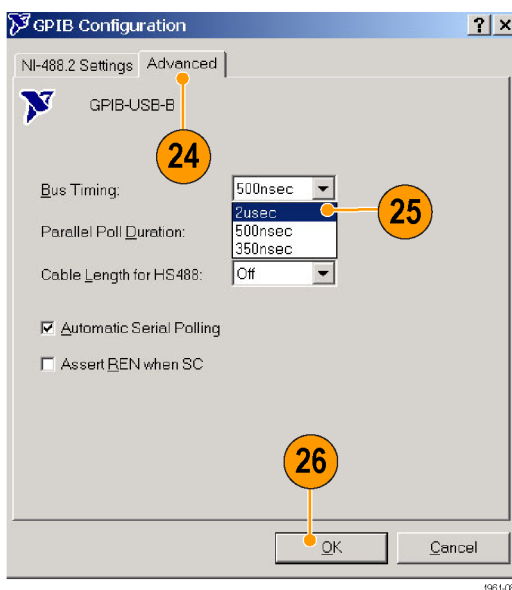


Configure the GPIB Address

27. Start the TDSHT3 software.

28. Click **Select**.


29. Click the **Sink** tab.

30. Select a Differential test, such as **Jitter Tolerance**.

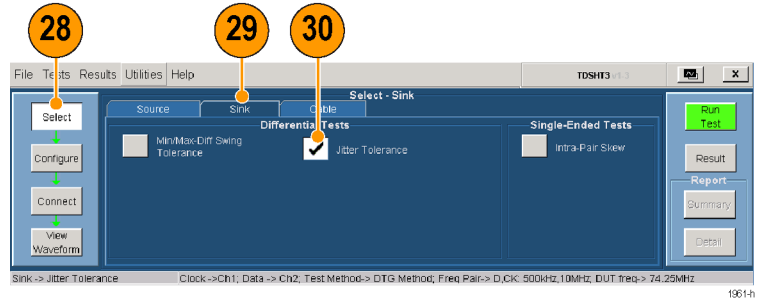

31. Click **Connect**.

32. Click **Signal Sources**.

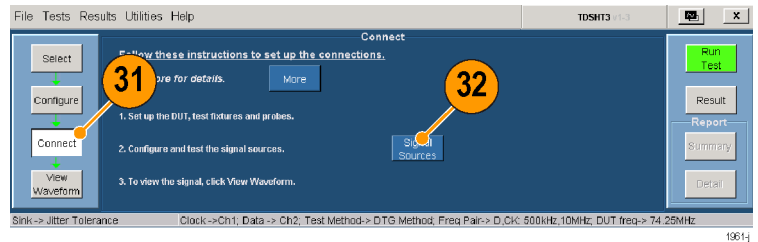

For the Tektronix DTG5274 or DTG5334 generator:

33. Click the **DTG** tab.


34. Click **GPIB**.

35. Click the **AWG** tab and repeat.

36. Click the **AFG** tab and repeat.

37. Click **Test Conn** and look for a message that the connection is successful.

38. Exit the TDSHT3 software and restart the oscilloscope.

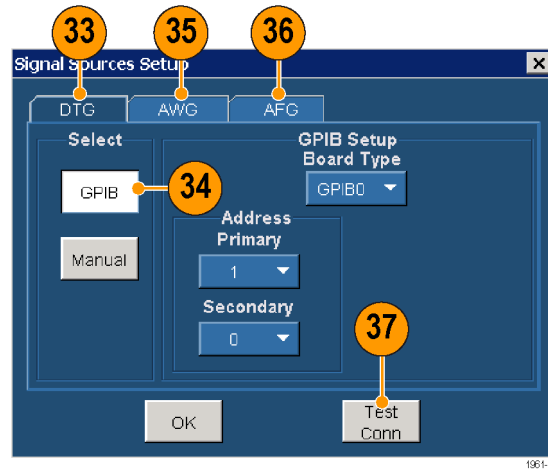

Index

A

- Acquisition, 10
- AFG setup, 32
- APP button, 11
- Application examples, 20
 - Cable tests: Eye Diagram, 29
 - Sink tests: Jitter Tolerance, 24
 - Sink tests: Min/Max-Diff Swing Tolerance, 22
 - Source tests: Select All, 20
- Auto Increment, 18
- AWG setup, 32

B

- Buttons, 7

C

- Cable
 - Eye Diagram test, 29
- Cable emulator, 26, 27, 28
- Cable Equalizer, 29
- Calibrate probes, 5
- Clear report, 18
- Client pane, 7
- Closing the application, 6
- Configure, 14
- Configure button, 13
- Configure test equipment, 32
- Configure the GPIB address, 38
- Connect, 14
- Connect button, 13
- Connect test equipment, 32
- Connections, 2
- CSV file, 18

D

- Detail, 19
- Detailed report, 18
- Device under test type, 7
- Documentation, v
- DTG setup, 32
- DTG5274, 38
- DUT type, 7

E

- Efficere Technologies, 2
- Error codes, 16
- Execution pane, 7
- Exit button, 6
- Exit the software, 6

F

- Factory defaults, 14
- File
 - Exit, 6
 - Preferences, 10
 - Run application, 3
- Fine button, 9

G

- General purpose knob, 9, 14
- Generate a report, 18
- Generator setup, 32
- Get acquainted with the application, 7
- GPIB, 38
- GPIB address, 38
- GPIB bus timing, 37

H

- Half Screen, 17
- HDMI standards conformance, iv
- Hide icon, 11
- Hide the application, 11
- How to
 - Install your software, 1
 - Make tests, 13
 - Operate the Application, 13

I

- Installation, 1
- Interface, 7

J

- Jitter Calibration, 26
- Jitter Tolerance test, 24

K

- Key features, iv
- Keyboard, 7
- Knob, 9, 14

M

- Make tests, 13
- Menu bar, 7
- Menus, 7
- Min/Max-Diff Swing Tolerance Test, 22
- Mouse, 7
- Multiple tests, 13

N

- NI-488.2 Software Configuration for DPO70000 series, 33
- NI-488.2 Software Configuration for TDS series, 33

O

- Oscilloscope general purpose knob, 14

P

- Pair, 18
- Position eye mask in center, 10
- Preferences, 10
- Print a report, 18
- Product description, iv

R

- Refresh Rate, 18
- Related documentation, v
- Remote control, 32
- Report File, 18
- Report summary, 18
- Resolution, 18
- Restore application, 12
- Result Details, 16
- Results, 16
- Results button, 13
- Return to the application, 11
- Run Test, 15

Run Test button, 13

S

Safety Summary, iii
Save As, 18
Select, 13
Select All, 13, 20
Select button, 13
Select multiple tests, 13
Selection pane, 7
Set preferences, 10
Signal Sources, 38
Sink

- Differential: Jitter Tolerance test, 24
- Differential: Min/Max-Diff Swing Tolerance Test, 22

Software upgrades, v
Source tab, 13
Source tests

- Select All, 20

Start the application, 3
Status bar, 7

T

TekVisa, 1
Test Conn, 38
Test equipment, 32, 36

- Connecting, 14
- Setups, 2

Test ID, 13
Test ID 5-3, 29
Test ID 8-5, 22
Test ID 8-7, 24
Test parameters

- Configuring, 14

Test results, 16
Tests

- Process flow, 13

Touch screen, 7
TPA-P-DI, 2
TPA-P-SE, 2

TPA-R-DI, 2
TPA-R-SE, 2
TPA-R-TDR, 2

U

Use the interface, 7

V

View test results, 16
View Waveform, 15
View Waveform button, 13
Virtual keyboard, 7, 14
Virtual keypad, 8