

Instructions



MTS4UP UPG MTS400 Series Software Upgrade 075-0912-00

www.tektronix.com



075091200

Copyright © Tektronix, Inc. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supercedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Contacting Tektronix

Tektronix, Inc.
14200 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
USA

For product information, sales, service, and technical support:

- In North America, call 1-800-833-9200.
- Worldwide, visit www.tektronix.com to find contacts in your area.

Kit Description

This document provides instructions for performing software and software key (dongle) upgrades on the following Tektronix products:

- MTS400 Series MPEG Test System
- MTS4SA MPEG Test System

NOTE. Only the software applications already installed on your MPEG test system will be available after the upgrade. If additional applications are required, contact your Tektronix representative.

This document supports Tektronix modification: ECR30701.

Products

MTS400 Series: All products
MTS4SA: All software versions

Minimum Tool and Equipment List

No tools are required to perform the upgrade.

Kit Parts List

Quantity	Part number	Description
1 EA	020-2654-xx	DOCUMENTATION KIT; ENGLISH GETTING STARTED MANUAL W/DOCUMENTATION CD-ROM; MTS400 SERIES
1 EA	063-3814-xx	SOFTWARE PKG; APPLICATION INSTALL CD-ROM; MTS400 SERIES
1 EA	NS	SOFTWARE KEY UPGRADE FLOPPY DISK
1 EA	071-1507-xx	MANUAL, TECH; USER, VOLUME 1 AND 2; MTS400 SERIES
1 EA	071-1726-xx	MANUAL, TECH; RELEASE NOTES; MTS400 SERIES
1 EA	075-0912-00	KIT INSTRUCTION; MTS4UP UPG

NS - Not Saleable

Upgrade Instructions

Perform the following steps to upgrade the MTS400 Series software:

Install Software Upgrade

1. Ensure that the instrument or PC to be upgraded is switched on and has completed the start-up process.
2. Insert the *MTS400 Series Application Install CD-ROM* supplied with this kit into the CD-ROM drive of the instrument or PC to be upgraded. The CD-ROM will autostart and display the Welcome screen shown in Figure 1.

NOTE. *If the CD-ROM fails to autostart, use Windows Explorer to locate and run the following file on the CD-ROM: start.exe.*

3. Click **Next** to initiate the upgrade process (see Figure 1).
4. Allow the installation process to proceed. The average installation time is approximately five minutes.

NOTE. *A number of dialog boxes are displayed during the installation process. Normally, no user intervention is required.*

5. When the upgrade installation is complete, the Update Complete screen is displayed as shown in Figure 2.
6. Select the **Yes, I want to restart my computer now** option, and then click **Finish**. The instrument or PC will shut down and then restart.

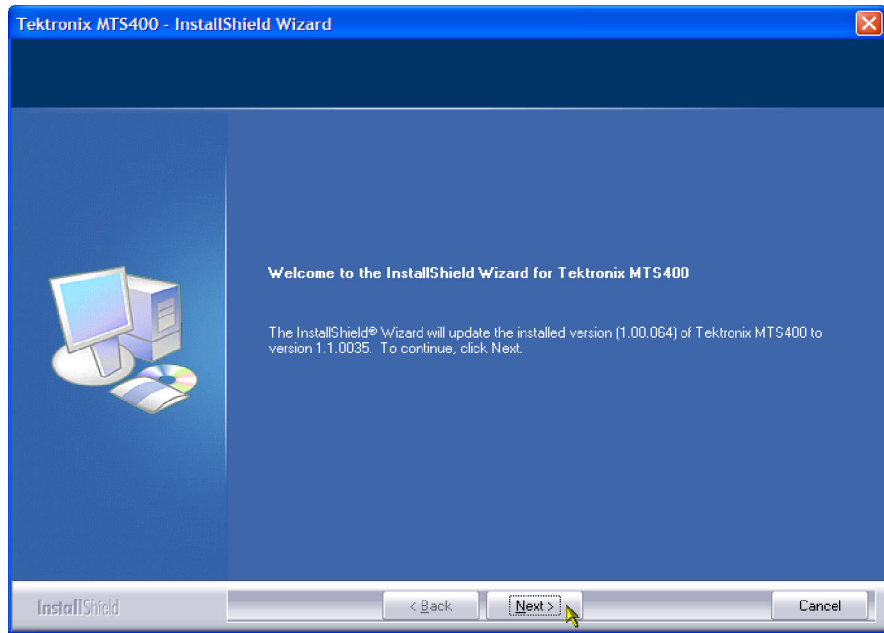


Figure 1: InstallShield Wizard welcome screen

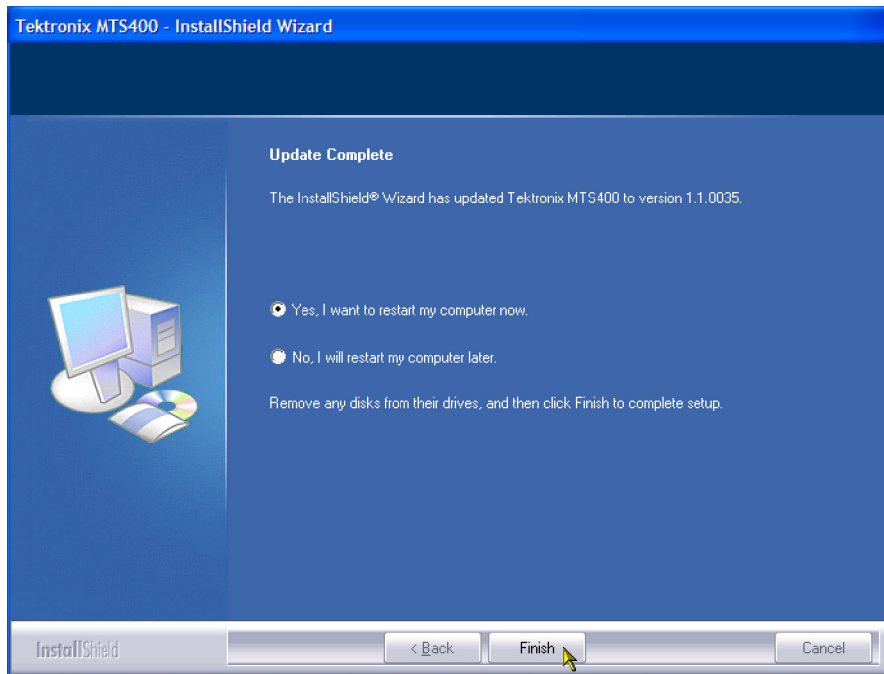


Figure 2: InstallShield Wizard update complete screen

Install the Software Key Upgrade

1. Ensure that the software key (dongle) is attached to your instrument.
2. Insert the *MTS400 Software Key Upgrade Floppy Disk* supplied with this kit into the floppy disk drive of the instrument or PC to be upgraded.
3. Using Windows Explorer, locate the floppy disk drive and double-click the following file: remoteupdate.exe.
4. The Tektronix Remote Update Utility screen will be displayed. Click **Perform Update** to start the update process (Figure 3).
5. The progress bar will show the status of the update.

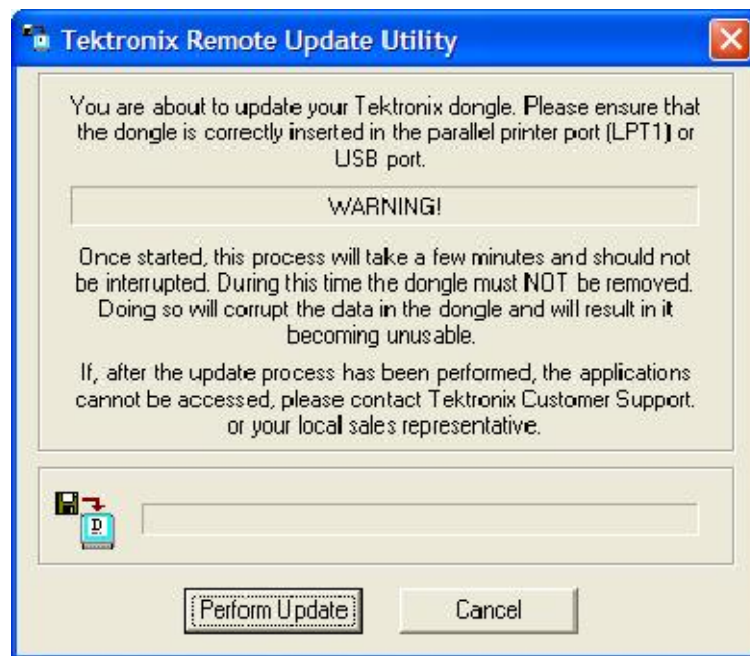


Figure 3: Tektronix Remote Update Utility screen

6. The remote update message box will indicate that the dongle has been reprogrammed (Figure 4). Click **OK** to complete the update.

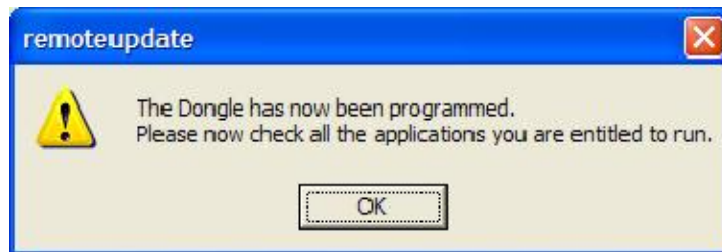


Figure 4: Remote Update message box

Verify Operation

To verify operation of the upgraded applications, open and close each installed application in turn.

If any licensed application fails to open correctly, contact your Tektronix representative.

❏ **End of document** ❏