

User Manual



VM5000 Option HD Automatic Video Measurement Set 071-1522-00

This document applies to firmware version 1.0
and above.

www.tektronix.com

Copyright © Tektronix, Inc. All rights reserved. Licensed software products are owned by Tektronix or its suppliers and are protected by United States copyright laws and international treaty provisions.

Use, duplication, or disclosure by the Government is subject to restrictions as set forth in subparagraph (c)(1)(ii) of the Rights in Technical Data and Computer Software clause at DFARS 252.227-7013, or subparagraphs (c)(1) and (2) of the Commercial Computer Software - Restricted Rights clause at FAR 52.227-19, as applicable.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supercedes that in all previously published material. Specifications and price change privileges reserved.

Tektronix, Inc., P.O. Box 500, Beaverton, OR 97077

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

WARRANTY

Tektronix warrants that the products that it manufactures and sells will be free from defects in materials and workmanship for a period of one (1) year from the date of shipment. If a product proves defective during this warranty period, Tektronix, at its option, either will repair the defective product without charge for parts and labor, or will provide a replacement in exchange for the defective product.

In order to obtain service under this warranty, Customer must notify Tektronix of the defect before the expiration of the warranty period and make suitable arrangements for the performance of service. Customer shall be responsible for packaging and shipping the defective product to the service center designated by Tektronix, with shipping charges prepaid. Tektronix shall pay for the return of the product to Customer if the shipment is to a location within the country in which the Tektronix service center is located. Customer shall be responsible for paying all shipping charges, duties, taxes, and any other charges for products returned to any other locations.

This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. Tektronix shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than Tektronix representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of non-Tektronix supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

THIS WARRANTY IS GIVEN BY TEKTRONIX IN LIEU OF ANY OTHER WARRANTIES, EXPRESS OR IMPLIED. TEKTRONIX AND ITS VENDORS DISCLAIM ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. TEKTRONIX' RESPONSIBILITY TO REPAIR OR REPLACE DEFECTIVE PRODUCTS IS THE SOLE AND EXCLUSIVE REMEDY PROVIDED TO THE CUSTOMER FOR BREACH OF THIS WARRANTY. TEKTRONIX AND ITS VENDORS WILL NOT BE LIABLE FOR ANY INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES IRRESPECTIVE OF WHETHER TEKTRONIX OR THE VENDOR HAS ADVANCE NOTICE OF THE POSSIBILITY OF SUCH DAMAGES.

Table of Contents

General Safety Summary	vii
Preface	ix
About This Manual	ix
Related Manuals and Online Documents	x
Contacting Tektronix	xi

Getting Started

Product Description	1-1
Key Features	1-1
Firmware Upgrade	1-3
Recommended Oscilloscope Probes	1-3
Installation	1-5
Unpacking	1-5
Checking the Environment Requirements	1-6
Connecting the Mouse	1-7
Powering On the Instrument	1-8
Shutting Down the Instrument	1-8
Creating an Emergency Startup Disk	1-9
Backing Up User Files	1-9
Installing Software	1-10
Connecting to a Network	1-11
Adjusting Display Contrast	1-12
Incoming Inspection	1-13
Self Tests	1-13
Functional Test	1-14
Options and Accessories	1-19
Options	1-19
Accessories	1-20

Operating Basics

Operating Basics	2-1
Input Signal Connection Requirements	2-1
Connecting Input Signals	2-2
The Matrix Test Signal	2-6
Starting the Application	2-7
The VM5000 Option HD Application User Interface	2-8
Measurement Steps Overview	2-9
Setting the Input Signal Format	2-9
Selecting Measurements	2-10
Setting the Measurement Run Operations	2-11
Taking and Viewing Measurements	2-13
Changing Line Number or Averaging on the Results Screen	2-14
Saving Measurement Setups	2-15
Recalling Measurement Settings	2-16
Saving Measurement Results (Reports)	2-17

Reference

Reference Overview	3-1
Menu Descriptions	3-3
The File Menu	3-3
The Configuration Menu	3-5
The Results Menu	3-8
The Utilities Menu	3-12
The Help Menu	3-13
Detailed Measurement Information	3-15
Matrix Signals and Line Numbers	3-15
Averaging	3-15
Measuring Channel Delay	3-16
Measuring Color Bars	3-18
Measuring Multiburst	3-19
Measuring Noise	3-21
Measuring Non Linearity	3-22
Measuring Sync	3-23

Appendices

Appendix A: Specifications	A-1
Appendix B: Performance Verification	B-1
Prerequisites	B-1
Required Equipment	B-1
VM5000 Option HD Tests	B-2
Appendix C: Remote Commands	C-1
Syntax	C-1
Remote Startup and Exit of the Instrument	C-3
Command Groups	C-4
Commands	C-8
AutoScale < setting >	C-8
ChannelDelayAll?	C-9
ChannelDelayAverage < samples >	C-10
ChannelDelayCh1Ch2?	C-11
ChannelDelayCh1Ch3?	C-12
ChannelDelayCh2Ch3?	C-13
ChannelDelayLine < linenumber >	C-14
ChannelDelaySet < setting >	C-15
ColorBarsAverage < samples >	C-16
ColorBarsLine < linenumber >	C-17
ColorBarsmVCh[1..3]?	C-18
ColorBarsmVCh[1..3]Val[1..8]?	C-19
ColorBarsSet < setting >	C-20
ColorSpace < colorspace >	C-21
DefaultSettings	C-22
Error < setting >	C-23
Execute < setting >	C-24
Format < format >	C-25
ID?	C-26
MultiburstAmpdBCh[1..3]?	C-27

MultiburstAmpdBCh[1..3]Val[1..6]?	C-28
MultiburstAverage < samples >	C-29
MultiburstFlagmVCh[1..3]?	C-30
MultiburstFreqCh[1..3]?	C-31
MultiburstFreqCh[1..3]Val[1..6]?	C-32
MultiburstLine < linenumber >	C-33
MultiburstSet < setting >	C-34
NoiseAmpdBCh[1..3]?	C-35
NoiseAmpmVCh[1..3]?	C-36
NoiseAverage < samples >	C-37
NoiseBW < bandwidth >	C-38
NoiseFilter < noisefilter >	C-39
NoiseLine < linenumber >	C-40
NoiseSet < setting >	C-41
NonLinearityAverage < samples >	C-42
NonLinearityLine < linenumber >	C-43
NonLinearityPctCh[1..3]?	C-44
NonLinearityPctCh[1..3]Max?	C-45
NonLinearityPctCh[1..3]Val[1..5]?	C-46
NonLinearitySet < setting >	C-47
OPComplete < setting >	C-48
RecallSettings < pathstring >	C-50
ReportGenerate < pathstring >	C-51
ReportMeasurements < setting >	C-52
ReportString < string >	C-53
RunMode < runmode >	C-55
SaveSettings < pathstring >	C-56
SetupAndOrRun < setuprunmode >	C-57
SyncAverage < samples >	C-58
SyncLevelsmV?	C-59
SyncLevelsmVVal[1..3]?	C-60
SyncLine < linenumber >	C-61
SyncSet < setting >	C-62
SyncTimes?	C-63
SyncTimesVal[1..7]?	C-64
Trigger < trigger >	C-65
WarningReportingMeasure < setting >	C-66
WarningReportingResults < setting >	C-67
WarningReportingSignal < setting >	C-68
Warning < setting >	C-69
Warning and Error Messages	C-70
Appendix D: Cleaning	D-1
Exterior Cleaning	D-1
Flat Panel Display Cleaning	D-1
Appendix E: Rebuilding the Hard Drive	E-1
Appendix F: Signal Source Disks	F-1
Baseband Test Signals CD	F-1
ATSC Transport Stream CD	F-3
Advanced TV Elementary Streams CD	
Standard Definition TV Elementary Streams CD	F-5
480 & 576 Line DVDs	F-7

Index

List of Figures

Figure 1-1: Instrument space requirements	1-6
Figure 1-2: Locations of VM5000 Option HD connectors	1-7
Figure 1-3: On/Standby switch location	1-8
Figure B-1: Signal output amplitude test hookup	B-3
Figure B-2: Amplitude accuracy test hookup	B-6
Figure B-3: Frequency accuracy test hookup	B-10
Figure B-4: Noise floor accuracy test hookup	B-12
Figure B-5: Channel delay match test hookup	B-14
Figure F-1: Using TG700 baseband test signals	F-2
Figure F-2: Using ATSC transport stream signals	F-4
Figure F-3: Using elementary stream signals	F-6
Figure F-4: Using DVD signals	F-7

List of Tables

Table 1-1: Recommended probes	1-3
Table 1-2: Instrument options	1-19
Table 1-3: Standard accessories	1-20
Table 1-4: Optional accessories	1-21
Table A-1: Video measurement specifications	A-1
Table A-2: Channel input and vertical specifications	A-2
Table A-3: Horizontal and acquisition system specifications	A-7
Table A-4: Trigger specifications	A-8
Table A-5: Display specifications	A-13
Table A-6: Input/output port specifications	A-13
Table A-7: Data storage specifications	A-14
Table A-8: Power source specifications	A-15
Table A-9: Mechanical specifications	A-15
Table A-10: Environmental specifications	A-16
Table A-11: Certifications and compliances	A-17
Table B-1: Required test equipment	B-1
Table B-2: Measured blanking to white levels	B-4
Table B-3: White bar measurement	B-7
Table B-4: Example white bar measurement values	B-8
Table B-5: Delay error measurements	B-15
Table C-1: Configuration commands	C-4
Table C-2: Miscellaneous commands	C-4
Table C-3: Reports commands	C-5
Table C-4: Results commands	C-5
Table C-5: Run commands	C-6
Table C-6: Settings commands	C-6
Table C-7: Setup commands	C-6
Table C-8: Warning messages	C-70
Table C-9: Error messages	C-71
Table F-1: Signal Source Disks	F-1
Table F-2: Available TG700 DNL signal format files	F-1
Table F-3: Available MXT100 .trp signal setup files	F-3

Table F-4: Available Advanced TV Elementary Streams	F-5
Table F-5: Available Standard Definition TV Elementary Streams	F-5
Table F-6: Available formats of DVD files	F-7

General Safety Summary

Review the following safety precautions to avoid injury and prevent damage to this product or any products connected to it. To avoid potential hazards, use this product only as specified.

Only qualified personnel should perform service procedures.

While using this product, you may need to access other parts of the system. Read the *General Safety Summary* in other system manuals for warnings and cautions related to operating the system.

To Avoid Fire or Personal Injury

Use Proper Power Cord. Use only the power cord specified for this product and certified for the country of use.

Connect and Disconnect Properly. Do not connect or disconnect probes or test leads while they are connected to a voltage source.

Ground the Product. This product is grounded through the grounding conductor of the power cord. To avoid electric shock, the grounding conductor must be connected to earth ground. Before making connections to the input or output terminals of the product, ensure that the product is properly grounded.

Observe All Terminal Ratings. To avoid fire or shock hazard, observe all ratings and markings on the product. Consult the product manual for further ratings information before making connections to the product.

Do Not Operate Without Covers. Do not operate this product with *metal* covers or panels removed.

Avoid Exposed Circuitry. Do not touch exposed connections and components when power is present.

Do Not Operate With Suspected Failures. If you suspect there is damage to this product, have it inspected by qualified service personnel.

Do Not Operate in Wet/Damp Conditions.

Do Not Operate in an Explosive Atmosphere.

Keep Product Surfaces Clean and Dry.

Provide Proper Ventilation. Refer to the manual's installation instructions for details on installing the product so it has proper ventilation.

Symbols and Terms

Terms in this Manual. These terms may appear in this manual:



WARNING. *Warning statements identify conditions or practices that could result in injury or loss of life.*



CAUTION. *Caution statements identify conditions or practices that could result in damage to this product or other property.*

Terms on the Product. These terms may appear on the product:

DANGER indicates an injury hazard immediately accessible as you read the marking.

WARNING indicates an injury hazard not immediately accessible as you read the marking.

CAUTION indicates a hazard to property including the product.

Symbols on the Product. The following symbols may appear on the product:



Preface

This is the user manual for the VM5000 Option HD Automatic Video Measurement Set. This manual focuses on the automatic video measurement functionality; it does not cover the oscilloscope functionality. Refer to *Related Manuals and Online Documents* for where to find information about using the oscilloscope functionality.

About This Manual

This manual is composed of the following chapters:

- *Getting Started* shows you how to configure and install your instrument and provides a functional check procedure.
- *Operating Basics*, using a highly-graphical approach, walks you through the basics of using the instrument user interface.
- *Reference* goes into more detail on the menu functions, understanding the measurements, and interpreting your results.
- *Appendices* provides additional information including instrument specifications, performance verification, remote command information, cleaning information, and signal source descriptions.

Related Manuals and Online Documents

This manual is part of a document set of manuals and online documentation. See the following list for other documents supporting operation and service.

Manual name	Description
<i>VM5000HD Automatic Video Measurement Set Online Help</i>	An integrated online help system, which can be accessed from the VM5000 Option HD help menu (located in the middle of the screen when the VM5000 Option HD application is open).
<i>TDS5000B Series Digital Phosphor Oscilloscope Quick Start User Manual</i>	A paper manual, which ships with the instrument, has information about installing and operating your instrument.
<i>TDS5000B Series Digital Phosphor Oscilloscopes Online Help</i>	An integrated online help system, which can be accessed from the oscilloscope platform help menu (located at the top right of the screen).
<i>Specifications and Performance Verification</i>	A .pdf only manual that includes both instrument specifications and the instrument performance verification procedure. You can access this manual from the instrument help menu, and it is installable from the <i>TDS5000B Series Product Software CD</i> .
<i>TDS5000B Series Oscilloscope Online Programmer Guide</i>	<i>Online help and .pdf versions are available from the TDS5000B Series Product Software CD.</i>
<i>TDS5000B Series Digital Phosphor Oscilloscopes Service Manual</i>	A description of how to service the instrument to the module level. This optional manual must be ordered separately.

Contacting Tektronix

Phone	1-800-833-9200*
Address	Tektronix, Inc. Department or name (if known) 14200 SW Karl Braun Drive P.O. Box 500 Beaverton, OR 97077 USA
Web site	www.tektronix.com
Sales support	1-800-833-9200, select option 1*
Service support	1-800-833-9200, select option 2*
Technical support	Email: techsupport@tektronix.com 1-800-833-9200, select option 3* 6:00 a.m. - 5:00 p.m. Pacific time

* **This phone number is toll free in North America. After office hours, please leave a voice mail message. Outside North America, contact a Tektronix sales office or distributor; see the Tektronix Web site for a list of offices.**



Getting Started

Product Description

This manual supports the VM5000 Option HD Automatic Video Measurement Set.

This chapter summarizes and highlights some of the key features of the instrument. Following this description are three sections:

- *Installation* shows you how to configure and install the instrument, as well as how to reinstall the system software included with the product.
- *Incoming Inspection* procedure verifies basic operation and functionality.
- *Accessories* lists the standard and optional accessories for this product.

Key Features

The VM5000 Option HD instrument is a high-performance solution for verification, debugging, and characterization of analog high-definition video signals. Key features include:

- Fast, accurate, and repeatable video measurements
- Fully automated, comprehensive component analog video measurements
- Supports HDTV, progressive, and PC-format component analog video (YPbPr and RGB)
- Acquisition bandwidth & high sample rates for HDTV signals
- Signal Source Disks for convenient test signal generator setup (see page F-1)
- Powerful automated measurement features and utilities
- Standard GPIB remote control capability
- MS Windows operating system, an intuitive graphical user interface, and online help for easy operation with minimal training time
- Video measurement accessories
- Extended documentation capabilities
- Complete oscilloscope functionality

Targeted to meet the needs of video professionals developing, testing, and manufacturing the next generation of Digital Television reception and play-out devices, the instrument incorporates the power, features, and functionality needed in R&D, QA, and Production Test applications. It enables manufacturers

to ensure that HDTV video signal quality is up to the challenge of today's high performance displays, as well as enables clear differentiation between input signal and display device impairments.

Applications include the following:

- R&D
- Compliance & certification testing
- Quality/audit testing
- Automated production test
- Off-air video systems testing

The VM5000 Option HD automates a variety of component analog video measurements utilized to verify the integrity and quality of HDTV video signals. It automatically assesses conformance of selected video signal parameters to applicable EIA-770-3, SMPTE - 274M, and 296M standards. It also automates measurement of other industry-standard video parameters that are utilized to quantify the performance of Digital Set-top boxes or other Consumer video reception and play-out devices with component analog interfaces.

By integrating automated measurement algorithms and a high-speed, wide bandwidth signal acquisition platform into one instrument, Tektronix offers a reliable means to make fast, objective, and accurate video measurements. Product verification activities that previously took hours or days to complete can now be completed in seconds or minutes. Offering near plug-and-play video measurement capability, even unskilled operators can reliably assess HDTV video output signal quality.

As a fully integrated video analyzer, the VM5000 Option HD offers simple configuration menu settings that can readily be recalled or copied, eliminating complicated oscilloscope set-ups, tedious manual measurements, and time-consuming results correlation exercises. Product quality is enhanced because reliable HDTV test results can be reliably generated, easily replicated with other VM5000 Option HD instruments, and readily communicated across a global engineering, supply, or sales organization.

The VM5000 Option HD offers intuitive Windows based configuration and measurement results menus for easy operation with minimal training time. A 10.4 in (264 mm) Color Display provides a bright, clear, and crisp display of waveforms and measurement results. Users can easily navigate through the logically arranged configuration and results menus, and make selections via radio buttons or an on-screen keyboard utilizing the included USB mouse.

Firmware Upgrade

Tektronix may offer firmware upgrade kits for the VM5000 Option HD instrument. Contact your Tektronix service representative for more information (see *Contacting Tektronix* on page xi).

Recommended Oscilloscope Probes

Table 1-1 lists the recommended oscilloscope probes to use when using the instrument as an oscilloscope.

Table 1-1: Recommended probes

Probe type	Tektronix probe
Passive, 10X, 500 MHz	P5050
Passive, 100X, 250 MHz, high voltage	P5100
Passive, 1000X, 100 MHz, high voltage	P6015A
Passive, 15 MHz, 1X	P6101B
Active, DC to 1.0 GHz, FET high speed digital, for CMOS/TTL technology	P6243
Active, DC to 1.5 GHz, FET high speed digital, for all technologies	P6245
Active, DC to 400 MHz, FET, high bandwidth differential	P6246
Active, DC to 1.0 GHz, FET, high bandwidth differential	P6247
Active, DC to 1.7 GHz, FET, high bandwidth differential	P6248
Active, 100 MHz, high voltage differential	P5205
Active, 50 MHz, high voltage differential	P5210
AC Current	P6021
AC Current	P6022
DC/AC Current	AM5030S
High Speed Current	CT-1/CT-2
Current, 250 KHz to 2 GHz, 50 Ω input, AC Only, for temporary in-circuit installation	CT-6
Current, DC to 50 MHz, 15 A DC	TCP202
Low Capacitance, 20X, 3 GHz	P6158
Current Measurement	TCPA3000
Current Measurement	TCPA4000
Differential Preamp	ADA400A
High Voltage Differential	P5200

Table 1- 1: Recommended probes (Cont.)

Probe type	Tektronix probe
Optical/Electrical Converter	P6701B
Optical/Electrical Converter	P6703B

Installation

This section addresses instrument installation:

- *Unpacking* on page 1-5
- *Checking the Environment Requirements* on page 1-6
- *Connecting the Mouse* on page 1-7
- *Powering On the Instrument* on page 1-8
- *Shutting Down the Instrument* on page 1-8
- *Creating an Emergency Startup Disk* on page 1-9
- *Backing Up User Files* on page 1-9
- *Installing Software* on page 1-10
- *Connecting to a Network* on page 1-11
- *Adjusting Display Contrast* on page 1-12



CAUTION. *Be sure to create your emergency startup disk as described on page 1-9. You may need that disk if you ever need to reinstall Windows 2000 on the instrument hard drive.*

Unpacking

Refer to the tables beginning on page 1-19 for a list of the options and accessories shipped with this instrument. Remember to fill out and send in the customer registration card.

Checking the Environment Requirements

Read this section before starting any installation procedures. This section describes site considerations, power requirements, and ground connections for your instrument.

Site Considerations

The instrument is designed to operate on a bench or on a cart in the normal position (on the bottom feet). For proper cooling, make sure that there is at least three inches (76.20 mm) of clearance on the left side of the instrument. If you need to access the instrument CD-RW drive, you will also need at least 5.1 inches (129.54 mm) of clearance on the right side of the instrument.

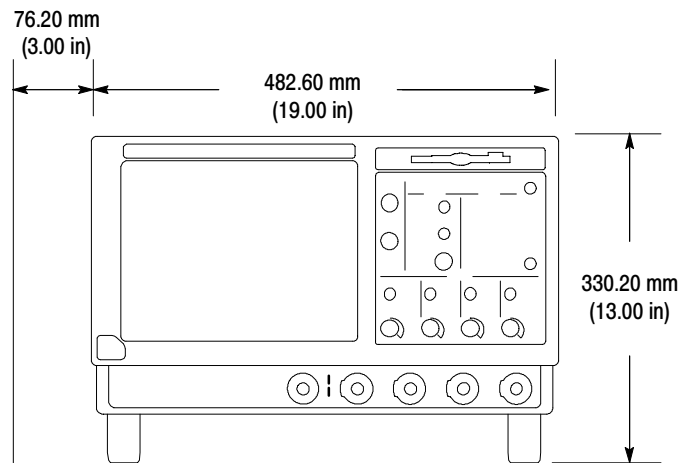


Figure 1- 1: Instrument space requirements



CAUTION. To ensure proper cooling, keep the bottom and left side of the instrument clear of obstructions.

Operating Requirements

The specifications in *Appendix A* list the power source, temperature, humidity, and altitude operating requirements for the instrument.

Connecting the Mouse

The instrument includes a USB (Universal Serial Bus) mouse. You can plug the mouse into any of the four available USB ports. The USB ports and other PC peripheral connection points are shown in Figure 1-2. Refer to the *TDS5000B Quick Start User Manual* for additional connection information.

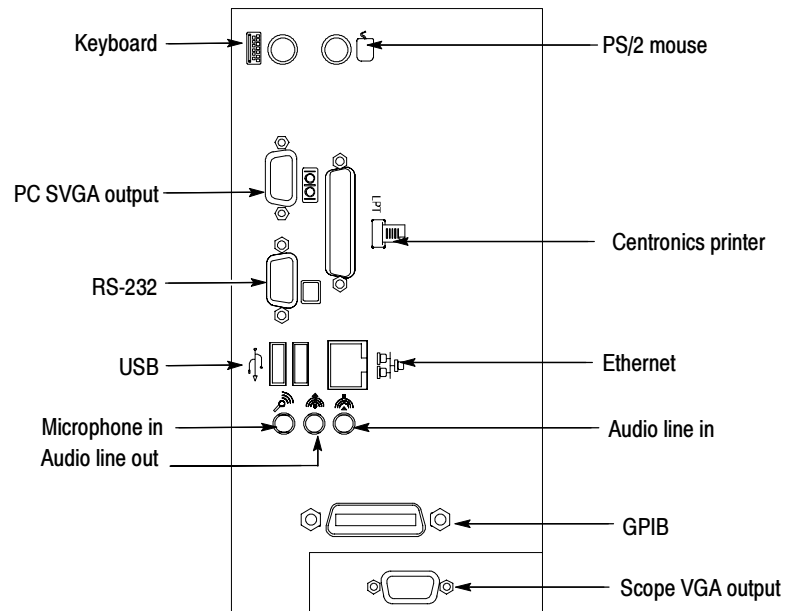


Figure 1-2: Locations of VM5000HD connectors

NOTE. For best performance, plug the USB devices directly into the USB connectors on the instrument chassis, rather than connecting the devices serially.

You can connect or disconnect USB mouse, keyboard, or other USB devices with the power on. If your USB mouse locks up, disconnect and reconnect the USB connector to restore normal operation.



CAUTION. To avoid product damage, shut down the instrument and disconnect the power cord from the power source before connecting any accessories other than USB devices. If the instrument front panel and/or touch screen does not respond, press the On/Standby switch for at least 5 seconds to cycle power. See Shutting Down the Instrument on page 1-8.

Powering On the Instrument

Follow these steps to power on the instrument for the first time.



CAUTION. *To ensure proper operation, connect the keyboard, mouse, and other accessories before applying power to the product the first time.*

1. Connect one end of the instrument power cord to the instrument and the other end to a power source.
2. Push the On/Standby switch to power on the instrument (see Figure 1-3 for the switch location).

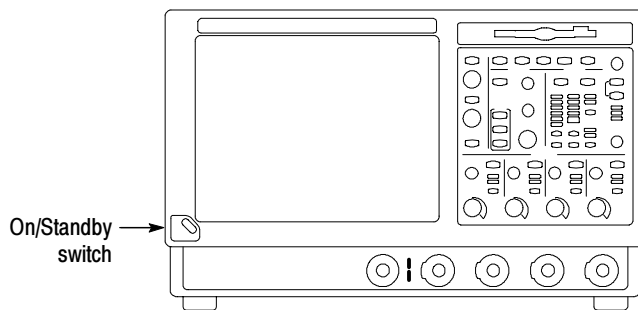


Figure 1-3: On/Standby switch location

Shutting Down the Instrument

To shut down the instrument, push the front-panel On/Standby switch. The instrument preserves settings and then starts a shutdown process (including a Windows shutdown) to put the instrument into standby mode. Avoid disconnecting the power cord or power source to shut down the instrument.

NOTE. *If you remove power instead of using the On/Standby switch to shut down the instrument, the instrument will be in the factory Default Setup when powered on the next time.*

If the shutdown process does not start immediately after pushing the ON/Standby switch, push and hold the On/Standby switch for up to 20 seconds to start the shutdown process.

To completely remove power to the instrument, push the On/Standby switch and then disconnect the power cord from the power source.

Creating an Emergency Startup Disk

Now that you have completed the basic installation process, you should create an emergency startup disk. The emergency startup disk contains basic files to restart your instrument in case of a major hardware or software failure. The disk also contains files that you can use to check and format the hard disk.



CAUTION. *Create this disk and store it in a safe place. It may help you recover your Windows 2000 installation without rebuilding the entire instrument hard disk.*

Follow these steps to create the emergency startup disk for a Windows 2000 instrument:

1. Minimize the instrument application by selecting **Minimize** in the File menu.
2. From the Windows taskbar, select **Start > Programs > Accessories > System Tools > Backup**.
3. In the Welcome display, click **Emergency Repair Disk**.
4. Insert a 3.5 in disk into the disk drive, and follow the on-screen instructions to create the startup disk.

Backing Up User Files

Always back up your user files on a regular basis. Use the Windows Backup tool to back up files stored on the hard disk. The Backup tool is located in the System Tools folder in the Accessories folder.

Use these steps to back up your files:

1. Exit the instrument application by selecting the File menu **Exit** command.
2. Click the Windows **Start** button.
3. Select **Programs > Accessories > System Tools > Backup**.
4. Use the Backup Wizard to select the items you want to back up and the destination. The destination can be the floppy drive or a third-party storage device over one of the side-panel ports.

Installing Software

The instrument system and application software is preinstalled at the factory. If you have to reinstall the software for any reason, refer to the instructions that accompany the CD-ROMs shipped with the instrument.

Software Release Notes

Read the software release notes (README.TXT) on the product software CD-ROM before performing installation procedures. This file contains additional information that supercedes other product documentation.

To view README.TXT, start the Windows Notepad accessory and open the file from the *VM5000HD Automatic Video Measurement Set Product Software* CD-ROM.

VM5000HD Remote Command Information

The GPIB programmer information is available in *Appendix C*.

Programmer information for the rest of the instrument functions is available as a .pdf file on the *TDS5000B Series Product Software CD-ROM*.

Desktop Applications

You can install desktop application software on the instrument. The instrument has been tested with the following software products installed:

- Microsoft Office 98 (Word, Excel, PowerPoint, and so forth)
- MathCad
- MATLAB

Other software products may be compatible but have not been tested by Tektronix. If the instrument malfunctions after you install software, uninstall the software and then reinstall the instrument software (if necessary) to restore proper operation.

Exiting the instrument Application. Before installing other desktop applications, exit the instrument application. To do this, select the **File > Exit** command.

Connecting to a Network

You can connect the instrument to a network to enable printing, file sharing, internet access, and other communications functions. Before you make the connection, do the following steps to enable network access to the instrument:

1. Begin with the instrument power off.
2. Attach a keyboard and mouse to the instrument.
3. Power on the instrument.
4. As the instrument begins to boot, press the keyboard **F2** key repeatedly until the message “Loading SETUP” appears.
5. In the BIOS Setup Utility, use the keyboard right-arrow key to highlight the **Advanced** menu at the top of the screen.
6. Use the arrow down key to highlight **Peripheral Configuration** in the Advanced screen, and then press **Enter**.
7. Use the arrow down key to highlight **LAN Device** in the Peripheral Configuration screen, and then press **Enter**.
8. Use the arrow up or down key to highlight **Enabled**, and then press **Enter**.

9. Press the **F10** key to save and exit. Confirm the Save of Configuration changes when you are prompted on screen.
10. Use the Windows network setup utility to define the instrument as a network client, and configure it for your network. You can find the network setup utility in the Windows **Start** menu if you select **Settings > Control Panel** and then double click **Network**. You should consult your network administrator for specific instructions to make these settings.

NOTE. *If you want to disable network access for the instrument, perform the above procedure, except substitute Disabled for the command listed in step 8. The instrument will boot faster with network access disabled.*

Adjusting Display Contrast

If you find that the instrument screen is too bright or too dark, use these steps to adjust the LCD display contrast to your preference. You must have a mouse attached to perform this procedure.

1. Right click with the mouse on the Windows desktop.
2. Select **Properties**.
3. Select the **Settings** tab.
4. Click **Advanced**.
5. Select the **Color** tab.
6. Adjust slider control for desired gamma setting. The screen brightness will change as you move the slider control.
7. Click **Apply**.
8. Click **OK**.

Incoming Inspection

This section contains instructions for performing a self test and functional verification of the instrument. These procedures verify that the instrument is operating correctly after shipment, but do not check product specifications.

If the instrument fails any test within this section, it may need service. To contact Tektronix for service, see *Contacting Tektronix* on page xi of *Preface*.

Make sure you have put the instrument into service as detailed in *Installation* starting on page 1-5.

Self Tests

This procedure uses internal routines to verify that the instrument functions and was adjusted properly. No test equipment or hookups are required.

Equipment required	None
Prerequisites	Power on the instrument and allow a 20 minute warm-up.

Perform these substeps to verify internal diagnostics:

1. *Display the system diagnostics menu as follows:*
 - a. If the instrument is in the toolbar mode, click **Menu** (far right toolbar button) to switch to menu bar mode.
 - b. From the Utilities menu, select **Instrument Diagnostics** to open the Instrument Diagnostics control window.
 - c. Ensure that ALL is selected from each drop-down list.
2. *Run the system diagnostics as follows:*
 - a. Disconnect all input signals from all four channels.
 - b. Click **Run** in the Instrument Diagnostics control window.

The internal diagnostics do an exhaustive verification of proper instrument function, taking five to fifteen minutes. When complete, the resulting status appears in the diagnostics control window.

3. *Verify that no failures are found and reported:* The instrument should pass all tests. If any failures occur, record the failure information and contact your local Tektronix service personnel for more information.
4. *Run the signal path compensation routine as follows:*

- a. From the Utilities menu, select **Instrument Calibration** to open the Instrument Calibration control window.
 - b. Click **Calibrate** to start the routine.
 - c. *Confirm signal path compensation returns passed status:* Signal path compensation may take up to ten minutes to run. Verify that the word **Pass** appears in the Status text box.
5. Click **Close** to exit the Instrument Calibration control window.

Functional Test

This procedure uses the output from a PC VGA video card to test the VM5000 Option HD application functionality.

Equipment required	VM5000 Option HD Sync Combiner cable assembly, Tektronix part number 012-1664-XX 75 Ω precision BNC terminations (3) BNC “T” connectors (3) A PC with a CD drive and a video graphics card capable of displaying an image at 1280 x 1024 at a 60 Hz refresh rate
---------------------------	---


NOTE. *These procedures verify that the application features operate. They do not verify that they operate within limits. Therefore, when the instructions in these functional tests call for you to verify that a signal appears on screen “that is about five divisions in amplitude” or “has a period of about six horizontal divisions,” and so on, do not interpret the quantities given as limits.*

Do not change the front-panel settings unless directed to by the procedure. If you change front-panel settings, you may obtain invalid results. In this case, redo the procedure from step 1.

When you are instructed to press a front-panel button or screen button, the button may already be selected (its label is lighted). If this is the case, it is not necessary to press the button.

1. Set the PC monitor display properties by doing the following steps:
 - a. Power on the PC and its monitor.
 - b. Position the cursor anywhere in the desktop background area and click the right mouse button to show the desktop menu.
 - c. Select **Properties** to show the Display Properties dialog box.
 - d. Select the **Settings** tab to show the display settings fields.
 - e. Set the Screen Area slider control to **1280 by 1024**.
 - f. Set the color field to **True Color (24 bit)**.
 - g. Select the **Advanced** button to open the advanced settings dialog.
 - h. Select the **Monitor** tab to display the monitor dialog.
 - i. Select **60 Hertz** in the Refresh Frequency list.
 - j. Select **OK** to dismiss the advanced dialog box. Depending on your Windows settings, the settings are applied immediately or you are requested to reboot your computer.
 - k. Select **OK** to apply the changes or to reboot your system.
 - l. Select **OK** to dismiss the Display Properties dialog box.
2. Set the PC to generate the test signal by doing the following steps:
 - a. Insert the *VM5000 Option HD Application Software* CD in the PC CD drive.
 - b. Start the Windows Paint program (**Start > Programs > Accessories > Paint**).
 - c. From within the Paint program, open the file <cd-drive>: **PCMatrix1280X1024P60.bmp**.
 - d. Select **View > View Bitmap** to display the file as a full-screen image (no window borders).
3. Turn off the monitor, and then disconnect the PC's monitor cable from the PC VGA video card output connector.
4. Connect the 15-pin connector on the Sync Combiner cable to the PC VGA video card output connector.

5. Connect the other end of the Sync Combiner cable to the VM5000 Option HD instrument inputs as shown.

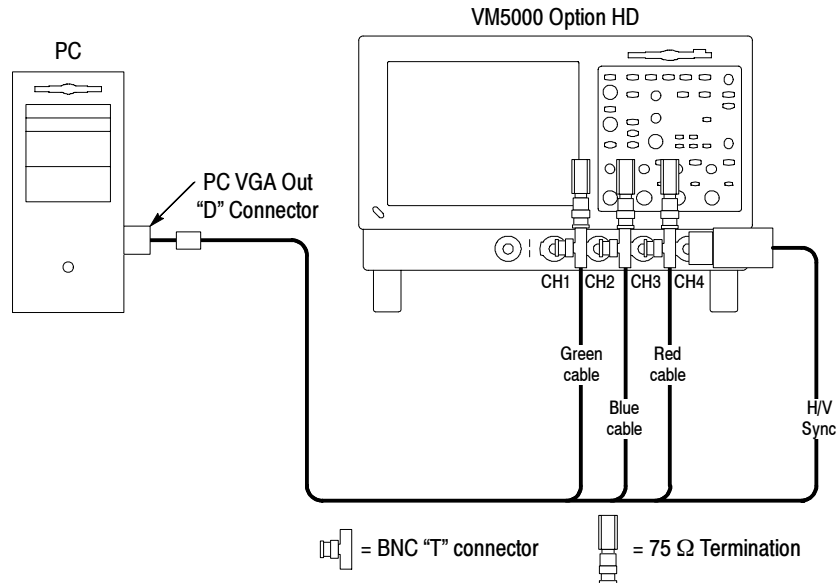

6. Power on the VM5000 Option HD instrument and wait for it to complete the power-on process.
7. Select **File > Run Application > VM5000HD** to display the VM5000 Option HD application window.
8. In the application window, select **File > Recall Default** to load the application default settings.
9. In the application window, select **Configuration > Format** to display the Format view.
10. Select the **SXGA/60** button.
11. In the application window, select **Configuration > Operation** to display the Operation view. Uncheck (turn off) All Measurement Warnings.
12. Select the **Channel 4** button in the Trigger area.

13. In the application window, select the **Run** button to start the application measurement process.



The instrument begins taking measurements and displays a Color bars measurement view listing measurement values similar to those shown below.

Results (mV)			
	Y/G	Pb/B	P r/R
White	692.24	684.13	686.69
Yellow	694.35	1.00	689.86
Cyan	695.61	686.12	1.64
Green	696.74	1.40	0.46
Magenta	2.03	686.63	688.50
Red	0.37	1.37	690.86
Blue	-0.17	687.41	1.86
Black	-0.43	2.12	0.20

Your actual measurement values will depend on your VGA output levels. They will vary from the nominals (700 mV and 0 mV) by about ± 50 mV, but you should observe the pattern shown in the screen capture above.

You have completed the VM5000 Option HD functional verification procedure.

Options and Accessories

This section lists the product options, standard accessories, and optional accessories that are available for the instrument.

Options

You can order the options shown in Table 1-2 with the instrument.

Table 1-2: Instrument options

Hardware	18	Touch-screen interface
	FHD	Front panel removable hard drive
	1K	Scope Cart
	655-4920-00	Thermal Printer-1P
Mounting	016-1946-XX	TDS5000B Series Rackmount Kit-1R
Software	SM	Serial Communications Mask Testing
	CP2	TDSCPM2-ANSI/ITU telecom pulse compliance software
	DVD	TDSDVD-Optical storage analysis software
	ET3	TDSET3-Ethernet compliance test software
	J2	TDSDDM2-Hard disk drive application software
	J3E	TDSJIT3E-Jitter and timing analysis software essentials
	JT3	TDSJIT3-Jitter and timing analysis software with Rj/Dj and BER
	PW3	TDSPWR3-Power measurement software
	USB	TDSUSBS-USB2.0 compliance test software only
Service	C3	Calibration Service 3 years
	C5	Calibration Service 5 years
	D1	Calibration Data Report
	with Option C3	Calibration Data Report 3 years
	with Option C5	Calibration Data Report 5 years
	R3	Repair service 3 years
	R5	Repair service 5 years

Accessories

This section lists the standard and optional accessories available. The accessories listed in Table 1–3 are shipped standard with the instrument.

Table 1-3: Standard accessories

Accessory	Part number
TDS5000B Series Digital Phosphor Oscilloscopes Quick Start User Manual	
English (Option L0)	071-1355-XX
French (Option L1)	071-1357-XX
German (Option L3)	071-1358-XX
Japanese (Option L5)	071-1356-XX
Korean (Option L9)	071-1359-XX
Russian (Option L10)	071-1401-XX
Simplified Chinese (Option L7)	071-1360-XX
Traditional Chinese (Option L8)	071-1361-XX
Accessory Pouch	016-1935-00
Keyboard	118-9402-00
Getting Started with OpenChoice Solutions Manual with CD	020-2513-XX
Important Documents Folder	Not orderable
Includes Certificate of Calibration documenting NIST traceability, 2540-1 compliance, and ISO9001 registration	
Front Cover	200-4651-00
Power Cord	
North America (Option A0)	161-0104-00
Universal Euro (Option A1)	161-0104-06
United Kingdom (Option A2)	161-0104-07
Australia (Option A3)	161-0104-05
240V North America (Option A4)	161-0104-08
Switzerland (Option A5)	161-0167-00
Japan (Option A6)	161-A005-00
China (Option A10)	161-0306-00
No power cord or AC adapter (Option A99)	
Optical Wheel Mouse	119-6936-XX
VM5000 Option HD Product Software CD-ROM	063-3768-XX

Table 1-3: Standard accessories (cont.)

Accessory	Part number
TDS5000B Series Product Software CD-ROM Includes: application, online help, TDS5000B Series Programmer Online Guide (GPIB online help and PDF), Specifications and Performance Verification PDF, release notes, VISA information, and other related documentation.	063-3692-XX
TDS5000B Series Operating System Restore CD-ROM	063-3693-XX
Optional Applications Software for Windows-Based Oscilloscopes CD-ROM and manuals	020-2450-XX
Signal Sources Disks	020-2507-XX
LabVIEW 30-day Evaluation Copy	020-2476-XX
MATLAB 30-day Evaluation Copy	063-3609-XX
One 500 MHz, 10x passive probe per channel	P5050
One BNC T Adapter, Male to 2 Females	103-0030-00
75 Ohm Coaxial Termination, BNC	011-0102-XX

The accessories in Table 1-4 were orderable for use with the instrument at the time this manual was published. Consult a current Tektronix catalog for additions, changes, and details.

Table 1-4: Optional accessories

Accessory	Part number
<i>TDS5000B Series Digital Phosphor Oscilloscopes Service Manual</i>	071-1362-XX
Transit Case	016-1937-00
Video Display Clamp	013-0278-XX
Thermal Printer Paper	016-1897-00
Probe Calibration, Compensation and Deskew Adapter. Requires a separate pulse generator.	067-0405-02
Power Deskew Fixture	067-1478-00
Extra Front Removable Hard Drive	065-0692-XX
P6101B 15 MHz 1X Passive Probe	P6101B
Extra P5050 500 MHz 10X Passive Probe	P5050
TCPA300, TCPA400 Series Current Measurement Systems (requires TCPA300 / TCPA400 style probe)	TCPA300 / TCPA400
AMT75 1 GHz 75 W Adapter	AMT75
AFTDS Differential Signal Adapter	AFTDS

Table 1-4: Optional accessories (cont.)

Accessory	Part number
K420 Scope Cart with mouse accessory tray	436-0317-XX
TDS5000 Series, VM5000 Option HD rackmount kit	016-1887-XX
GPIB cable (3.3 ft / 1 m)	012-0991-01
GPIB cable (6.6 ft / 2 m)	012-0991-00
Centronics cable	012-1214-00



Operating Basics


Operating Basics

This section provides basic information about using the VM5000 Option HD. More detailed measurement information can be found in the *Reference* section.

Input Signal Connection Requirements

Use only 75 Ω coaxial cables to connect the video device under test to the VM5000 Option HD instrument.

Install the included 75 Ω terminations between the end of the coaxial cables and the instrument input channels, using the included BNC “T” connectors. For accurate frequency response measurements, it is important to attach the “T” connector directly to the VM5000 Option HD input channel BNCs.

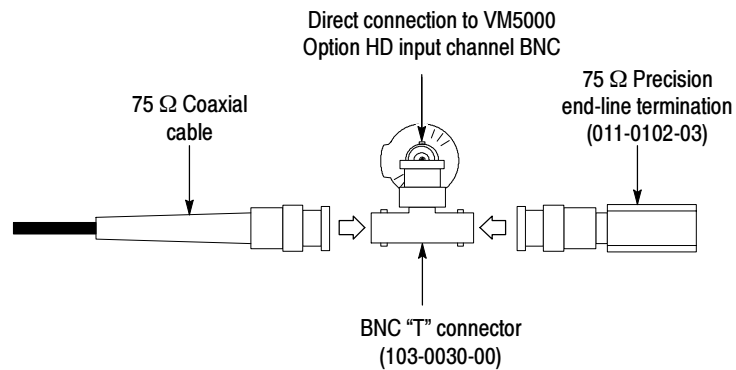


Connecting Input Signals

Use the following diagrams to determine the optimum input signal setup for your measurement needs.


3-Wire Video with Composite Sync, Setup 1

Use this setup for testing 3-wire component analog video signals (Y/G, Pb/B, Pr/R) with the composite sync signal on Y/G, triggering the instrument on channel 1 (the default trigger setting). This setup provides the most accurate frequency response information, but limits noise measurement on Y/G to -65 dB (30 MHz noise bandwidth).

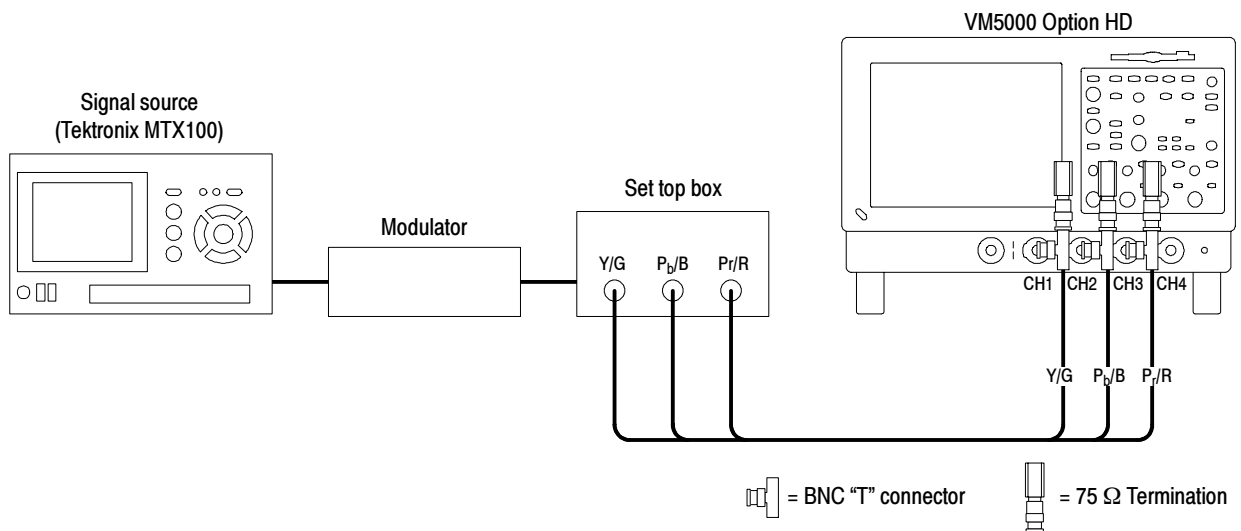

3-Wire Video with Composite Sync, Setup 2


Use this setup for testing 3-wire component analog video signals (Y/G, Pb/B, Pr/R) with the composite sync signal on Y/G, triggering the instrument on channel 4. This configuration provides more accurate low-level (below -60 dB at 30 MHz bandwidth) noise measurements than setup 1. Frequency response measurements on the Y/G will be degraded by approximately 0.04 dB (0.5%) at 30 MHz due to the additional loading from the CH4 input.

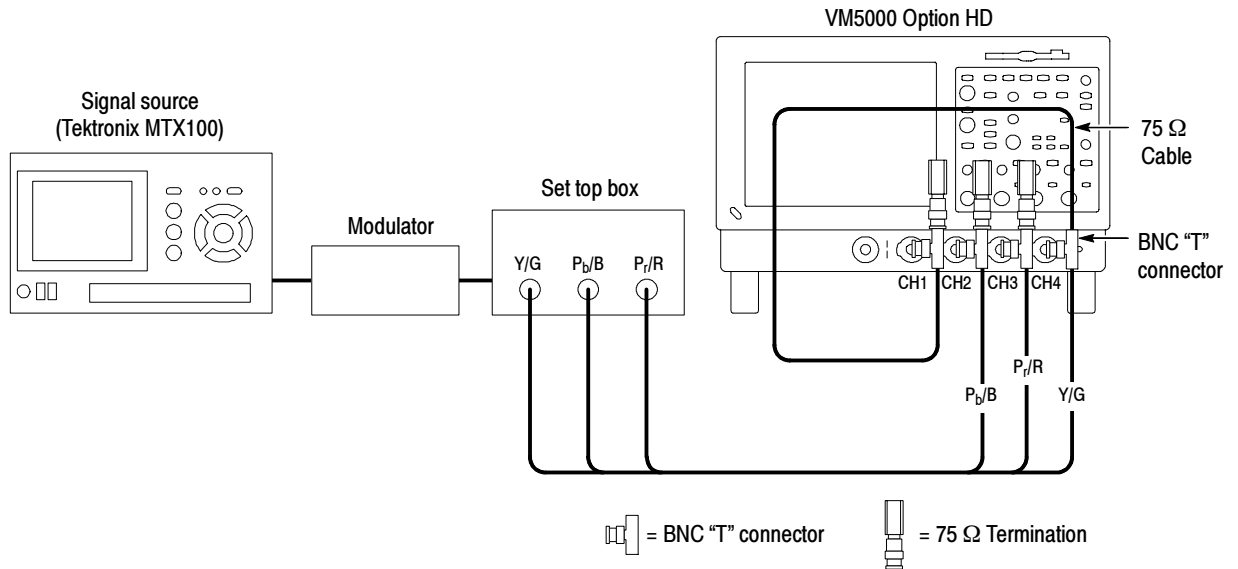

NOTE. Be sure to set the trigger channel to channel 4; the default trigger channel is channel 1. If you do not change the trigger setting (Configuration > Operation), you will see signal warning messages and be unable to take measurements.

4-Wire Video with Separate Composite Sync


Use this setup for testing 4-wire component analog video signals (Y/G, Pb/B, Pr/R) with the composite sync signal on a separate output line. For CH4, termination is optional. For CH4 only, you can use no termination or a 75 Ω termination of lower accuracy than the 75 Ω terminations that are provided with the instrument.

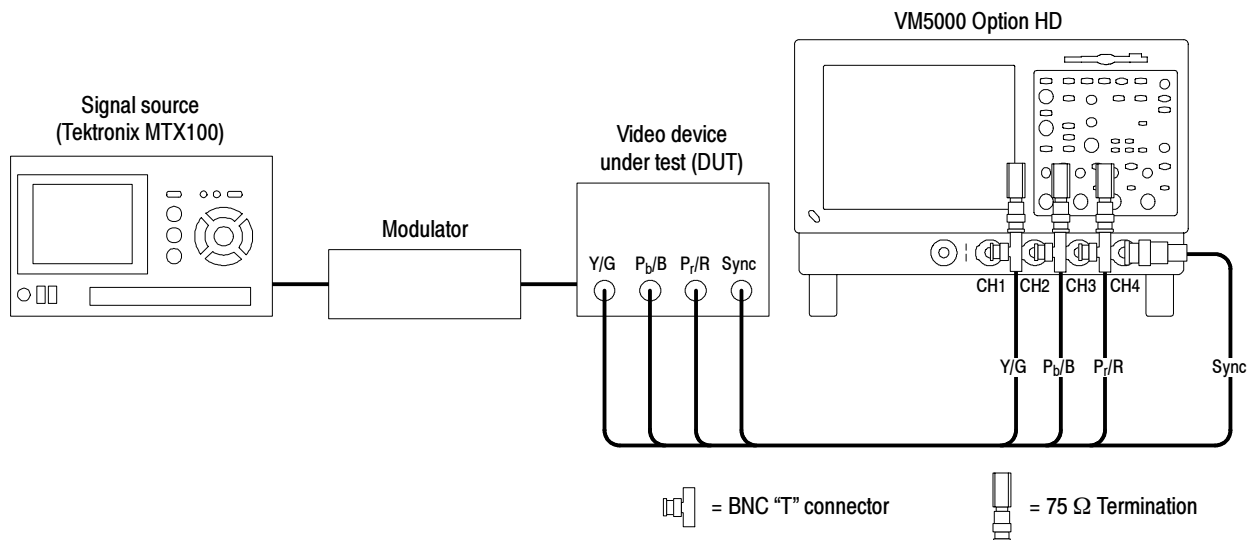

NOTE. Be sure to set the trigger channel to channel 4; the default trigger channel is channel 1. If you do not change the trigger setting (Configuration > Operation), you will see signal warning messages and be unable to take measurements.

VGA PC Video Card Signal Measurement Setup


Use this setup for testing 3-wire component analog video signals (Y/G, Pb/B, Pr/R) without the composite signal on Y/G, and triggering the instrument on channel 4. Use the special VGA sync combiner cable to connect the PC video card to the instrument. (Use this setup for the Functional Tests beginning on page 1-14.)

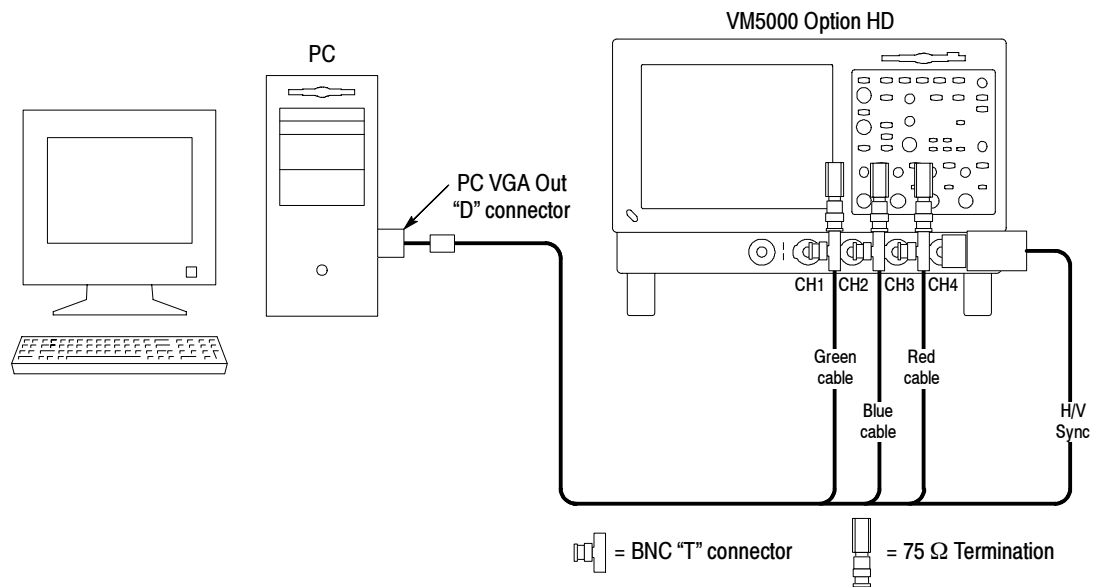

NOTE. Be sure to set the trigger channel to channel 4; the default trigger channel is channel 1. If you do not change the trigger setting (Configuration > Operation), you will see signal warning messages and be unable to take measurements.

The Matrix Test Signal

The Matrix test signal, shown below, is provided with the accessory Signal Source Disks provided with this product. It incorporates all analog HD video signal requirements into different line numbers within one test pattern field. Using a single test pattern eliminates the need to change test signals when doing different measurements. All you need to change is line numbers. Use the setup file (.vmset) that matches the format of the Matrix test signal you are using; this provides appropriate line numbers as default settings for each measurement type. See page F-1 for a full description of the files on the Signal Source Disks.

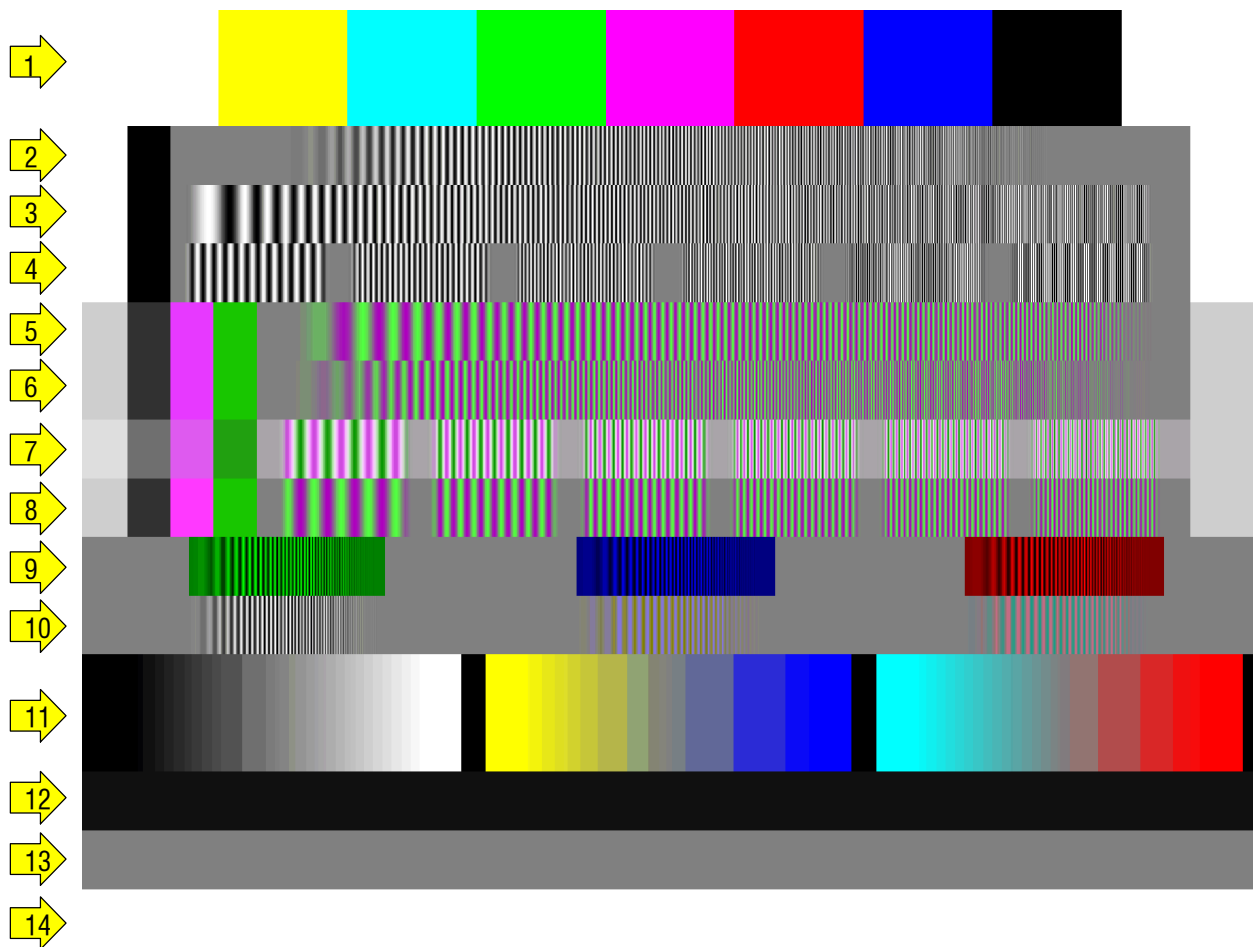


Signal	Format	Signal	Format	Signal	Format
1. Color bars	All	6. Sweep	YPbPr	11. Valid ramp	All
2. Sweep	RGB	7. 30 MHz MB	YPbPr	12. Flat field: 0% black	All
3. Sweep	RGB	8. 15 MHz MB	YPbPr	13. Flat field: 50% grey	All
4. Multiburst	RGB	9. Windowed sweep	RGB	14. Flat field: 100% white	All
5. Sweep	YPbPr	10. Windowed sweep	YPbPr		


Starting the Application

Make sure you have set up the input signal sources before taking measurements (see page 2-9).


1. Power on the instrument. The instrument displays the default main screen.

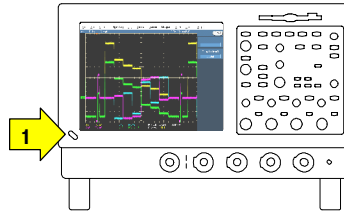

2. In the menu bar, select **File > Run Application > VM5000 Option HD**.

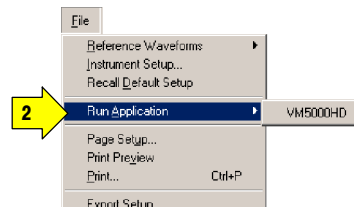


The instrument reduces the waveform area to the upper half of the display, and opens the VM5000 Option HD application in the lower half of the display.

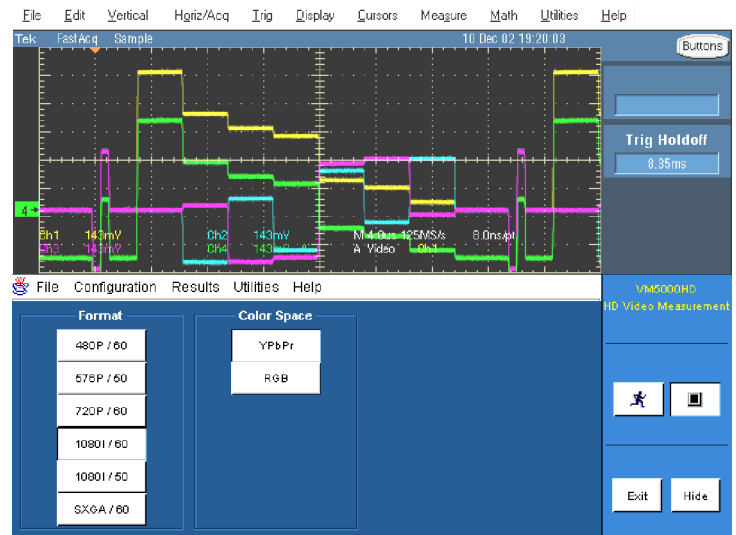


The VM5000 Option HD Application User Interface

1. Menu bar: Selects setting controls and results information to display in the Application view.
2. Application view: Displays configuration controls and measurement results.

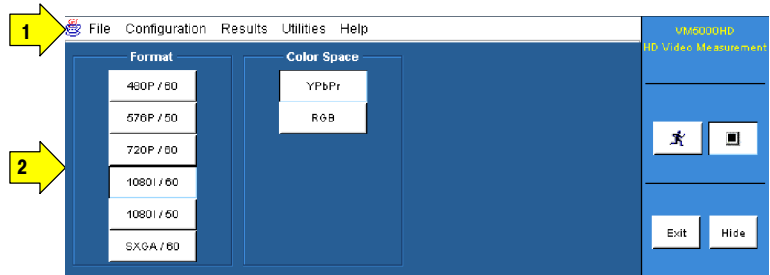

3. Run Button: Sets up, starts taking measurements, and displays results.
4. Stop button: Halts the measurements.

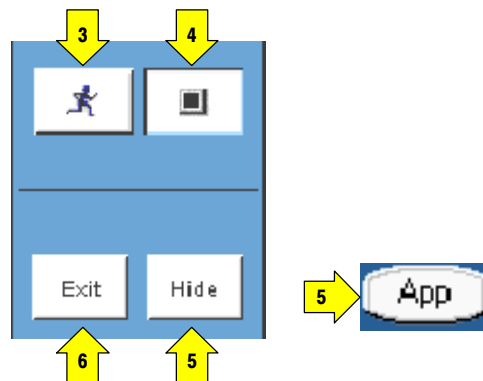

5. Hide button: Restores the main display to full-screen and hides the application window behind the main display.

To restore the application window after hiding it, select the **App** button on the main display.

To access the MS Windows desktop (for viewing reports), select **Hide**. In the main display, select **File > Minimize**, and then select the application **Hide** button again.


6. Exit button: Exits (closes) the application and returns the instrument to the default main display.

Measurement Steps Overview


1. Set the input signal format standard (such as 1080i/60) and color space (Y Pb Pr or RGB) by using the Configuration > Format menu (page 2-9).
2. Select one or more measurements to take by using the Configuration > Measurements menu (page 2-10).
3. Set the measurement run operations, such as run mode and trigger channel, by using the Configuration > Operation menu (page 2-11).
4. Select the Run button to take and view measurements (page 2-13).
5. Save measurement results by using the Utilities > Generate Reports menu (page 2-17).

Setting the Input Signal Format


1. Select **Configuration > Format**.



The application opens the Format view.

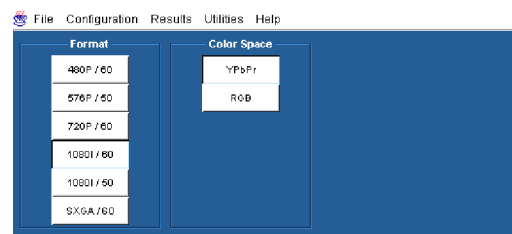


2. Select the appropriate video format for the signal you are measuring.
3. Select the appropriate color space type for the signal you are measuring.

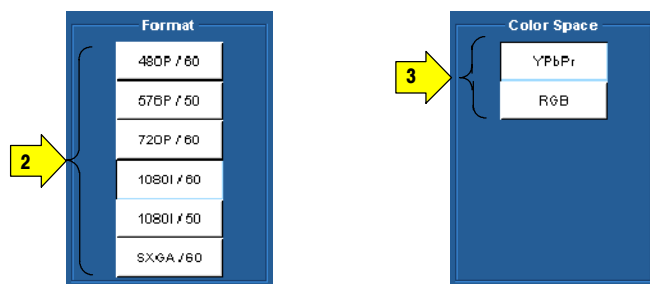


Selecting Measurements

1. Select **Configuration > Measurements**.




2. Select from one to six measurements, in any combination.

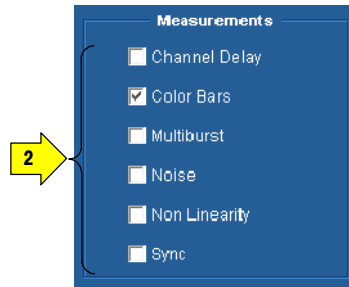


Setting the Measurement Run Operations


1. Select **Configuration > Operation**.



The instrument displays the Operation view. These settings control how the instrument sets up and acquires measurements when you select the Run button.

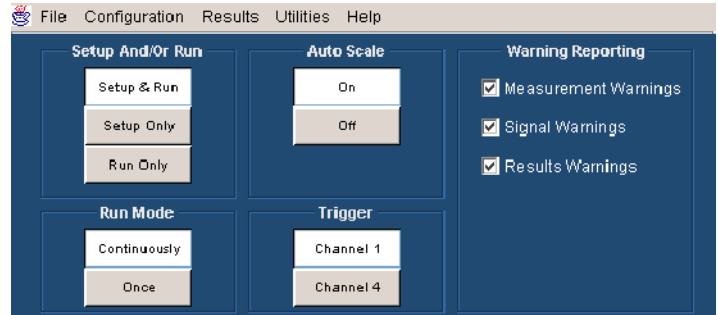


2. Select how the instrument sets up and runs measurements.

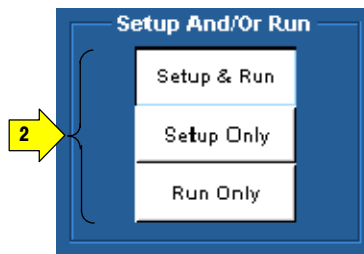


- **Setup & Run** configures the instrument settings and takes a measurement, for each selected measurement, and for each measurement acquisition. Use this when taking multiple measurements that require different instrument setups.
- **Setup Only** configures the instrument for a measurement but does not take the measurement. Use this to set up customized settings. Try out your settings by pressing the Run button, make adjustments as needed (for example, change the horizontal scale), and then select the Run button again. Once you are satisfied with your customized setup, use the Run Only setting to collect results.
- **Run Only** takes a measurement using the existing instrument configuration. Designed for taking measurements with custom settings (see Setup Only description above).

3. Select how the application acquires measurements (run mode).

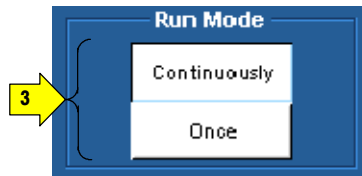


- **Continuously** continually takes measurements. You must select the Stop button to stop measurements.
- **Once** takes each selected measurement the number of times determined by the averaging setting, then stops taking measurements.

4. Enable or disable waveform autoscaling. Auto Scaling adjusts the vertical scale units so that the input signals fill the graticule as much as possible. Auto Scaling occurs once for each selected measurement. Refer to page 3-7 for details.

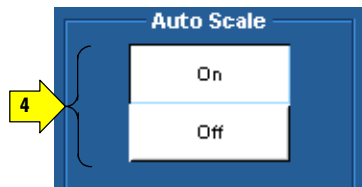

5. Select which instrument channel has the sync signal for triggering.

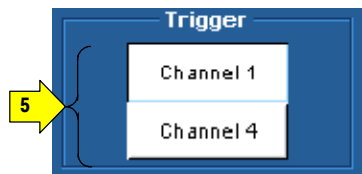

If you use the wrong trigger channel (and Signal Warnings is on), you will get a signal warning. See the setup diagrams and trigger requirements on page 2-2.

6. Select which warning messages to display.




See page 3-7 for more information.


Taking and Viewing Measurements

Make sure you have selected a signal format, selected one or more measurements, and configured the run options before taking a measurement.


1. Select the **Run** button.




The instrument begins taking measurements and displays the measurement results view for the most recently-selected measurement result.

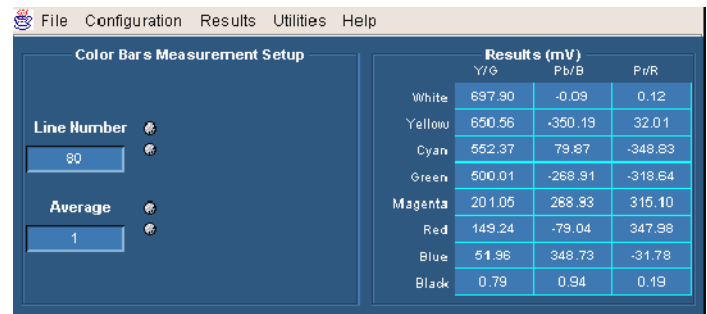


2. To view the results for other measurements, select the measurement from the Results menu. For example, to view the Sync measurement results, select **Results > Sync**.

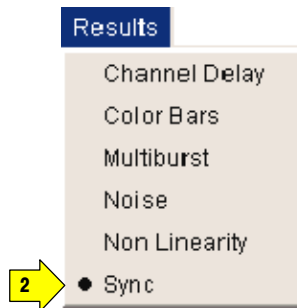

The instrument displays the selected measurement results. You can only display results for measurements that are selected in the Format > Measurements view.

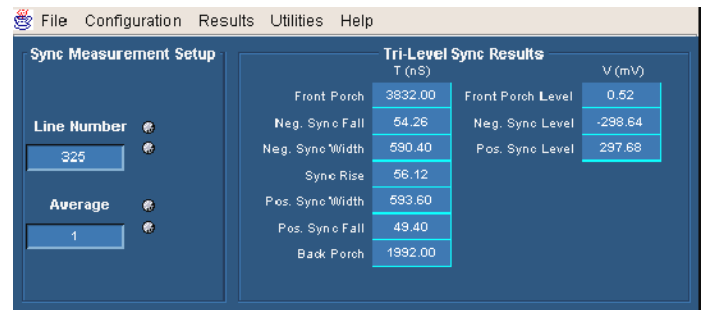


3. If you set the run operation to Continuously, press the **Stop** button to stop taking measurements.




Changing Line Number or Averaging on the Results Screen


1. Select a measurement from the Results menu. For example, select **Results > Sync**.

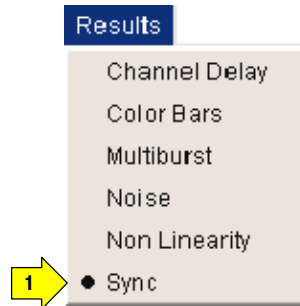

The instrument displays the selected measurement results.


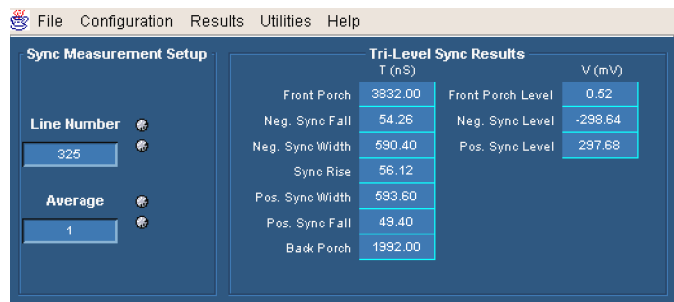


2. You can change the video signal line number and the number of measurements to average before displaying results. The instrument stops measuring, changes results to dashes, and uses the new settings at the start of its next measurement cycle. Refer to page 3–8 for information on line numbers and averaging.




To change a value, select the field and enter a value by keyboard. You can also change values using one of these methods:

3. Select the keypad icon to the left of the field to display a virtual keyboard to enter values using the touch screen.
4. Use the indicated general purpose knob to change the value.

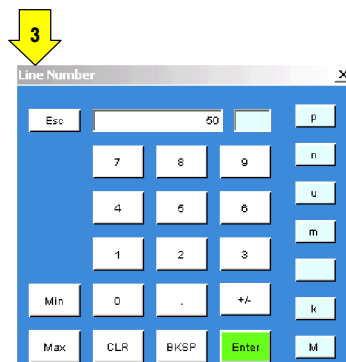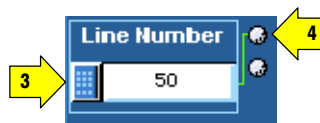


Saving Measurement Setups


1. Select **File > Save**.




The application displays the Save dialog. The default save location is C:\VM5000 Option HD.

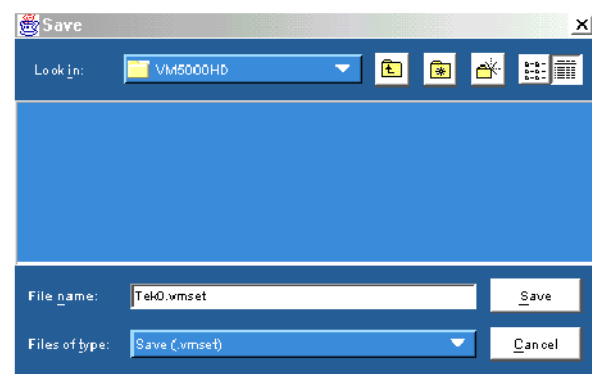

2. Select the **Look In** list to navigate to a different directory other than the default save location.

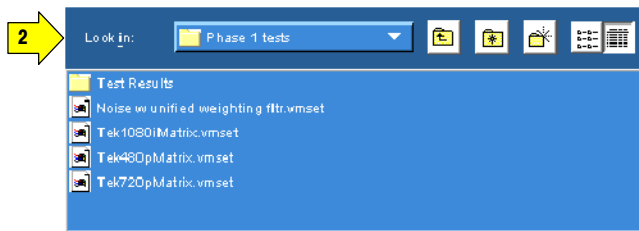


3. Enter a file name in the File Name field. The instrument offers an available file name (or you can choose your own). It automatically appends .vmsset to the file name of measurement setup files.




4. Select **Save** to save the measurement settings to the specified location and file name.

Recalling Measurement Settings


1. Select **File > Recall**.



The application displays the Recall dialog and lists all instrument setting files that are present in the default C:\VM5000 Option HD directory.

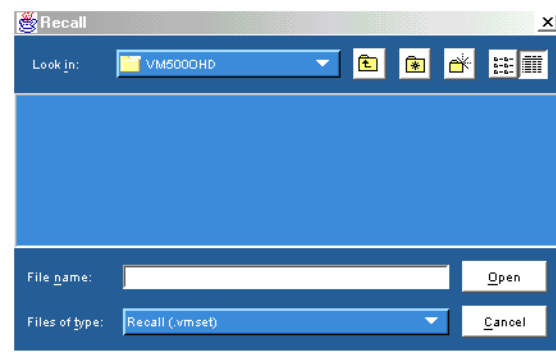

2. Select the **Look In:** button to navigate to a different directory other than the default location (if desired).
3. Select a file from those listed.

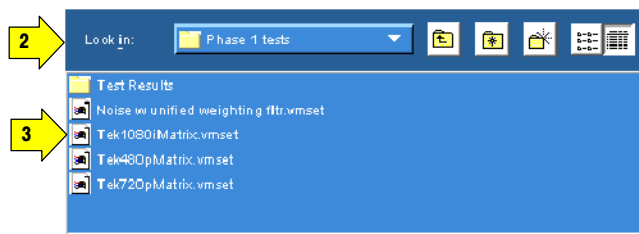

4. Enter a file name in the **File name:** field or select a file from the list.
5. Select **Open** to load the settings file and configure the instrument.




Saving Measurement Results (Reports)

You can use the Generate Report function to save your measurement results.


1. Select **Utilities > Generate Report.**



The instrument displays the Utilities Report Generator view.

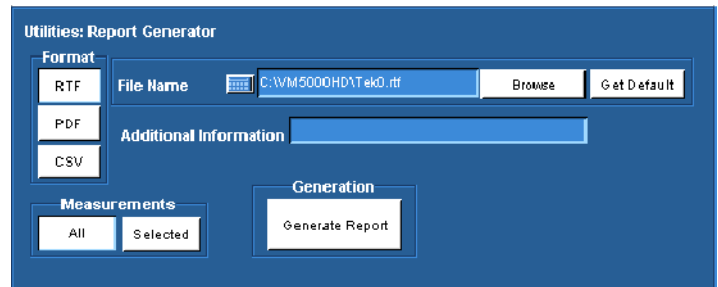


2. Select a report format. Which format to select depends on what you want to do with the measurement results.



- **RTF:** Use RTF (Rich Text Format) to create results data that you can incorporate into documents.
- **PDF:** Use PDF (Portable Document Format) to create PDF files of the measurement data for distribution and viewing. PDF is especially useful for ensuring that the results cannot be altered.
- **CSV:** Use CSV (Comma-Separated Values) to create results data that you can insert into spreadsheets or math software in which you can create limits to verify that your results are within expected range.


3. Use the File Name field to specify where you want to save the report. Use the Browse button to navigate to a specific location. Use the Get Default button to reset the file name to the default location and name for the selected format.



4. Use the Additional Information field to add notes into the report file. You can enter up to 46 characters. For example: “Serial Number 123456789012 tested by J. Smith”




5. Use the Measurements buttons to select which measurements to save to a report.



- **All:** Creates a report with all the measurements you have run since starting the application which have valid results in the results panels.
- **Selected:** Creates a report with only the measurements that are currently selected in the Configuration> Measurements screen and that have valid results in the results panels.

6. Select Generate Report to save the measurement results to the specified format and location. All selected measurements are saved together in a single file; each measurement has its own area in the report.

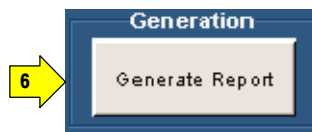



Reference

Reference Overview

This chapter provides a detailed description of the VM5000 Option HD instrument menus and measurements.

- Menu descriptions. The table below lists the top level of the instrument menus and the sections in this chapter that document those menus. The menu descriptions include high-level descriptions of the six measurements.
- Measurement details. Refer to page 3-15 for an in-depth description of each of the six measurements.

Overview of menu descriptions

Menu	Submenu	Function	Page
File	Recall Default	Restores default application measurement settings	3-3
	Recall	Recalls (loads) saved application measurement setups	
	Save	Saves (writes) saved application measurement setups	
	Minimize	Minimizes the application to the Windows task bar	
Configuration	Format	Sets the input signal format	3-5
	Measurements	Selects measurements to take	
	Operation	Sets measurement runtime options	
Results	Channel Delay, Color Bars, Multiburst, Noise, Non Linearity, Sync	Displays the selected measurement results Adjusts individual measurement settings	3-8
Utilities	Generate Report	Saves measurement results to specified file format	3-12
Help	Help Topics	Opens the VM5000 Option HD online help system	3-13
	About VM5000HD	Displays the application version number	

Menu Descriptions

The following tables list each menu item and its functions. Items in **bold face** are the default application settings when first starting the application or after doing a Recall Default operation.

The File Menu

Recalling a setup file changes the configuration; current measurements will stop and results appear as dashes.

NOTE. To avoid losing unsaved measurement results, generate a report before recalling the default setup or another .vmset setup file.

Menu item	Function	Setting or field	Description
Recall Default	Recalls (loads) and applies the default application measurement settings.		
Recall			Recalls (loads) and applies application measurement settings from the specified file.
	Look in	Drop-down menu VM5000HD	Sets the directory to list in the File list area.
	File list area	Filename list field	Lists directories (folders) and setup files that are in the current directory (as set by Look in).
	File name	Text entry field	Field in which to enter an application setup file to load and apply. You can also double-click on a file name in the File list area to enter the name in the File Name field.
	Files of Type	Drop-down menu .vmset	Lists the valid setup file types. The only valid entry is .vmset. To get valid test results, be sure to choose the appropriate setup file for the signal source you are using. For example, for the Option SS Matrix signal source file Tek1080iMatrix.trp, be sure to use the Tek1080iMatrix.vmset setup file. The correct .vmset setup file will have the correct line numbers for each measurement as the defaults.
	Open		Loads and applies the specified instrument setting file.
	Cancel		Closes (exits) the Recall dialog and does not load or apply any settings.
Save	Saves (writes) the current application measurement settings to the specified file name and directory.		
	All of the Save dialog functions are the same as those for the Recall dialog except for the Save button.		

Menu Descriptions

Menu item	Function	Setting or field	Description
	Save		Saves the application measurement settings to the specified file directory (as set by Look in) and file name (as entered in the File name field) as file type .vmset.
Minimize	Minimizes the application to the Windows task bar.		

The Configuration Menu

All the selected measurement results will appear as dashes any time you change any the following configurations:

- Format
- Color Space
- Trigger

If you change a configuration while running a measurement or a setup, the measurement or setup will stop.

Recalling a setup file changes the configuration; current measurements will stop and results appear as dashes.

NOTE. To avoid losing unsaved measurement results, generate a report before changing any configuration parameters other than selecting measurements or turning warnings on or off.

Menu item	Function	Setting or field	Description
Format	Sets the video input signal format. The Format setting also affects other measurement settings, such as the video signal line number to use when taking measurements.		
	Format	480P / 60 576P / 50 720P / 60 1080I / 60 1080I / 50 SXGA / 60	Sets the input signal format.
	Color Space	YPbPr RGB	Sets the input signal color space type.
Measurements	Selects the video signal measurements to take. You can select from one to six measurements, in any combination.		
	Measurements	Channel Delay Color Bars Multiburst Noise Non Linearity Sync	<p>Selects from one to six measurements, in any combination. When you click the Run button, the selected measurements will be taken. The results of the measurements you select here will be included in any report you generate, if you select Utilities > Generate Report and then set Measurements to Selected.</p> <p>For a detailed discussion of measurements, refer to page 3-15. For a high-level overview of measurements, refer to page 3-8.</p>

Menu Descriptions

Menu item	Function	Setting or field	Description
Operation	Sets the measurement runtime options, including test run mode, input trigger channel, and warning message display.		
	Setup And/Or Run	Setup & Run	Automatically configures the instrument settings and takes a measurement, for each selected measurement, and for each measurement acquisition. Use this when taking multiple measurements that require different instrument setups.
		Setup Only	Configures the instrument for a measurement but does not take the measurement. Use this to set up customized settings. Customized settings might include changes to the instrument Horizontal or Vertical front panel controls to display and measure a non-supported video signal standard. Try out your settings by pressing the Run button, make adjustments as needed (for example, change the horizontal scale), and then select the Run button again. Once you are satisfied with your customizations, use the Run Only setting to collect results.
		Run Only	Run Only Uses the current instrument and application settings to take a measurement. Use this for taking measurements after setting up the instrument using Setup Only to create custom settings.

Menu item	Function	Setting or field	Description
	Run Mode	Continuously	Continuously continually takes measurements, in the order the measurements are listed in the Configuration > Measurements view. You select the Stop button to stop measurements.
		Once	Takes each selected measurement the number of times required for the averaging you have selected, and then stops taking measurements.
	Auto Scale	On Off	<p>Enables or disables waveform Auto Scaling. Auto Scaling adjusts the vertical scale units so that the input signals fill the entire graticule as much as possible without going out of range. Auto Scaling occurs once for each selected measurement.</p> <p>If you are doing only one type of measurement and change the amplitude of the signal, you may need to auto-scale again: set Auto Scale to Off and then to On again. If you don't re-auto-scale in this way, then you might get bad results, inefficient use of the dynamic range, or your signal may be out of range.</p> <p>If you are using custom instrument settings (for example, changes to Vertical or Horizontal settings made from the instrument front panel or from remote GPIB commands), you should turn Auto Scaling Off.</p> <p>If you are sure your signal is set up correctly and you want to make further measurements in a high speed production line, set Auto Scale to Off.</p>
	Trigger	Channel 1 Channel 4	Sets the input channel on which to trigger the instrument. Refer to the setup illustrations starting on page 2-2 for appropriate trigger channel settings.
	Warning Reporting	Measurement Warnings Signal Warnings Results Warnings	<p>Sets which warning messages to display on the instrument screen while taking measurements. All warning messages are enabled by default. Clear a warning message check box to disable displaying warning messages.</p> <p>Measurement warnings include the most general information about potential problems in making the measurement. Signal warnings appear if signals are absent or change. If there are some valid results, Results warnings let you know if some of the displayed results may not be valid. A Results warning message box also tells you which types of test results are included in a report you have just generated.</p> <p>If warnings are selected, message boxes may appear on screen, requiring you to click OK. To avoid interruptions to your testing, disable all of the Warning reporting, especially if you are using the GPIB interface.</p>

The Results Menu

If you change the Line Number or Average values for any measurement, or if you change the Filter configuration in the Noise measurement, then that the changed measurement will stop running and its results will change to dashes.

All the selected measurement results will appear as dashes any time you change any the following configurations:

- Format
- Color Space
- Trigger

If you change a configuration while running a measurement or a setup, the measurement or setup will stop.

The Average setting interacts with your choices for the Run Mode. For example, if you select Once for the Run Mode and you set the averages to 2, then when you select the Run button, each selected measurement will run twice and then stop. On the other hand, if you select Continuously for the Run Mode and 2 averages, then when you select the Run button, each selected measurement will run twice, display results, and then continue running and updating the results for every two measurements.

If you are using Matrix signal source files from the standard-accessory Signal Source Disks, be sure to use the appropriate matching .vmset setup file, if necessary, to get the correct default values for Line Number for each measurement. See page F-1 for more information about the signal source files.

For a detailed discussion of measurements, refer to page 3-15.

Menu item	Function	Setting or field	Description
Channel Delay	Measures the time variation between the three video channels. The instrument measures the crossings of all three channels.		
	Channel Delay Measurement Setup	Line Number	Sets the video signal line number to measure. The default value depends on the input signal format as set by Configuration > Format, and is based on using the Matrix test signal to generate the test signal.
		Average: 1	Sets the number of acquisitions over which to calculate an average measurement value.
Results (ns)		Displays the time variation, in nanoseconds, from channel 1 to channel 2, from channel 2 to channel 3, and from channel 3 to channel 1.	
Color Bars	Measures all eight color levels of the three video channels. The instrument locates and measures the back porch signal of each channel, and then measures each channel's color values relative to that channel's back porch level.		

Menu item	Function	Setting or field	Description
	Color Bar Measurement Setup	Line Number	Sets the video signal line number to measure. The default value depends on the input signal format as set by Configuration > Format, and is based on using the Matrix test signal to generate the test signal.
		Average: 1	Sets the number of measurements acquisitions over which to calculate an average measurement value.
	Results (mV)		Displays eight color values, in mV, for each channel (24 measurements total).
Multiburst	Measures the video channel frequency response and amplitude. The instrument measures the flag pulse on each channel to determine and measure the six burst frequencies with the largest amplitude.		
	Channel Delay Measurement Setup	Line Number	Sets the video signal line number to measure. The default value depends on the input signal format as set by Configuration > Format, and is based on using the Matrix test signal to generate the test signal.
		Average: 1	Sets the number of measurements acquisitions over which to calculate an average measurement value.
Multiburst Measurement Results		Displays the flag signal value (in mV) for each channel in the first display row. The following six rows list the frequency (in MHz) and amplitude (in dB) of each channel, for each of the six burst signals.	

Menu Descriptions

Menu item	Function	Setting or field	Description
Noise	Measures video signal noise using one of three filter settings.		
	Noise Measurement Setup	Line Number	Sets the video signal line number to measure. The default value depends on the input signal format as set by Configuration > Format, and is based on using the Matrix test signal to generate the test signal.
		Average: 1	Sets the number of measurements acquisitions over which to calculate an average measurement value.
	Filter	Off	Disables (turns off) all noise signal filtering. Use this setting to measure broadband noise without any filtering.
		Unified Weighting	Enables (turns on) unified weighting noise signal filtering. Use this setting to measure noise with the psychovisual weighting established by CCIR Recommendation (Rec) 576-2, adjusted for the selected video format.
		Unweighted w/ Bandwidth	Enables (turns on) unweighted noise signal filtering and activates the filter bandwidth field. Use this setting to remove high frequency noise from your signal.
		Bandwidth Hz	Sets the bandwidth filter cutoff frequency. Selecting Unweighted activates this field. The default value depends on the input signal format as set by Configuration > Format.
Results		Displays the noise measurement results for each channel in dB (relative to peak white) and mV.	
Non Linearity	Measures channel signal linearity based on a ramp or five-step linearity test signal. If using a ramp signal, the instrument divides the ramp signal into five values to determine the equivalent step values. The instrument then measures the bottom, individual step, and top values of the test signal, and compares these values to a nominal value to determine the percent of deviation of the test signal from the nominal signal.		
	Non Linearity Measurement Setup	Line Number	Sets the video signal line number to measure. The default value depends on the input signal format as set by Configuration > Format, and is based on using the Matrix test signal to generate the test signal.
		Average: 16	Sets the number of measurements acquisitions over which to calculate an average measurement value.
	Results (%)		Displays the percent of deviation of the test signal from a nominal signal value, as a percentage, for each step on each channel.
Sync	Measures the sync signal timing and voltage values. The instrument measures the sync signal rise and fall times (at the 10% and 90% signal amplitude levels) and the sync pulse width (at the 50% signal amplitude level) to determine the signal timing values.		
	Sync Measurement Setup	Line Number	Sets the video signal line number to measure. The default value depends on the input signal format as set by Configuration > Format, and is based on using the Matrix test signal to generate the test signal.

Menu item	Function	Setting or field	Description
		Average: 1	Sets the number of measurements acquisitions to take and then calculate the average measurement value.
	Tri-Level Sync Results		Displays the sync signal timing values in ns, and the signal levels in mV.

The Utilities Menu

NOTE. To avoid losing unsaved measurement results, generate a report before recalling a .vmset setup file or changing any configuration parameters other than selecting measurements or turning warnings on or off.

Menu item	Function	Setting or field	Description
Generate Report	Save (write) measurement results in three popular data formats.		
	Format	RTF	Use RTF (Rich Text Format) to create results data that you can incorporate into documents.
		PDF	Use PDF (Portable Document Format) to create PDF files of the measurement data for distribution and viewing.
		CSV	Use CSV (Comma-Separated Values) to create results data that you can insert into spreadsheets or math software.
File Name		Text entry field C:\VM5000HD\Tek0.rtf	Field in which to enter the report file name.
		Browse	Selects the location to which to write (save) the report.
		Get Default	Sets the report write directory to the default location and name (C:\VM5000HD\Tek0.rtf).
Additional Information		Text entry field	Adds a brief note into the report file. You can enter up to 46 characters.
Measurements		All	Creates a report with all the measurements that you have run since starting the application.
		Selected	Creates a report with only the measurements that are currently selected in the Configuration > Measurements screen.
Generation		Generate Report	Writes the specified measurement data in the selected report format to the specified location.

The Help Menu

Menu item	Function	Setting or field	Description
Help Topics			Opens the VM5000 Option HD online help window that provides you with application information on your instrument screen.
About VM5000HD			Displays a VM5000 Option HD dialog that contains the application software version number.

Detailed Measurement Information

For a high-level procedure for how to take a measurement, refer to page 2-9.

For a high-level overview of all the measurements, refer to the table beginning on page 3-8.

The following information applies to all measurements.

Matrix Signals and Line Numbers

The matrix signals provided with the standard-accessory Signal Source Disks (see page F-1) provide appropriate signals for all measurements. See the Readme.txt files on the disks for extensive information about the files provided.

When using Tektronix supplied matrix test signals, if a .vmset file is provided for that format of matrix test signal, be sure to use the default line numbers in the associated .vmset file (File > Recall...). Otherwise, under most circumstances, use the instrument default line numbers (File > Recall Defaults).

For example, when using the ATSC transport stream file:

Tektronix1080iATSCMatrix.trp,

you should select File > Recall... and then navigate to where you have saved the setup file:

Tektronix1080iATSCMatrix.vmset.

The line numbers in this setup file may be used for all formats including 1080i, 720p, and 480p in both YPbPr and RGB.

For the equivalent matrix test signal .DNL from a Tektronix TG700 video generator, use the default settings.

Averaging

The higher the averaging, the lower the variance of the measurement in the presence of noise or other transient signal components. Set the averaging higher if you would like to reduce the fluctuations in the measurement results.

The instrument averages results, not input waveforms. (If, on the other hand, the Noise waveforms were averaged instead of the Noise results, the noise results would appear lower than they should. Because the instrument averaging results, this problem is avoided.)

Measuring Channel Delay

Channel delay measurement is used to verify relative timing of the three channels of video. Nominal channel delay is zero between all channels. Deviations from zero correspond to decreased video quality. For example, the greater the delay between channels, the more likely the edges in video will be perceived as distorted. Using a narrow band signal, the delay at a particular frequency band can be measured and thus group delay can be obtained.

In addition, channel delay is a function of relative cable lengths for each of the channels. Thus, if a splitter is used at the video source output, delay due to cable length mismatch can be measured.

Signal Source

You can use the matrix signal, or you can use a signal with high cross-correlation between each pair of channels to be tested. The default signal is the multiburst signal used for multiburst measurement, but many other types of signals can be used, including sweeps and even some live program material. If the cross-correlation is high enough for at least one pair of channels, the measurement results will display. Otherwise, running the measurement will result in “---” for each channel. If warnings are enabled, low correlation between channels will result in associated warnings.

Interpreting Results

A positive number indicates that the first signal arrives later than the second signal. For example, Y to Pb delay of 4.03 ns means that the signal in the Y channel is delayed 4.03 ns relative to Pb. However, the signals may contain distortions, which create different delays for different portions of the video line. In such a case, the measurement result is the delay compensation required to maximize the cross-correlation of the second channel with the first, generally giving a weighted average of the various delays. For narrow band signals, the delays at a particular frequency band may be measured. An ensemble of such measurements may be collected to develop a portrait of group delay.

If the signals of the three channels are highly mutually correlated (which is the case if the signals are reconstructed well and free of distortions other than delay), the “loop” delay will be approximately zero:

$$\text{Delay1} - \text{Delay2} + \text{Delay3} = 0, \text{ where}$$

Delay1 is Y to Pb or G to B

Delay2 is Y to Pr or G to R

Delay3 is Pb to Pr or B to R

The more the loop delay deviates from zero, the less the three signals mutually correlate. High loop delay corresponds to different types of signals among the three channels, because of differences either in distortions or in the inherent source signal (as in some live program material, for example). Loop delay greater than 5ns will generate a warning if warnings are enabled.

**How Results are
Calculated**

The maximum cross-correlation of transitions is found between each pair of channels. The location of the maximum is the delay in time. Generally, one may think of the calculation of the delay as the average match of transitions, weighted by the amplitude of each transition.

Measuring Color Bars

Measuring GBR color bars from a set-top-box can be used to verify the correct colorimetry conversion. Likewise, conversion from 1080i/720p to 480p colorimetry in YPbPr can be verified. The Color Bars measurement also can be used to check individual channel gain. In addition, it can be used as a crude check of linearity since severe clipping or other non-linear distortions will alter the measurement results from the ideal.

Signal Source You can use the matrix signal, or you can use a signal with all eight valid color bars on the line. There is no requirement for the order of the bars except for the bias that black will be searched after (to the right of) blue. Each of the bars should be at least 1/24 of the active line time in duration.

Interpreting Results The Color Bars measurement measures the amplitude level (relative to back porch) of each of the 8 colors (white, yellow, cyan, green, magenta, red, blue, black) for each active channel. Therefore, this measurement makes 8 measurements on 3 channels for 24 total measurements. The software assumes Y is on Channel 1, Pb is on Channel 2, and Pr is on Channel 3.

NOTE. *Some signals intentionally reverse or change the order from the traditional color bar test signal order. Since the bars are measured regardless of order, if channel inputs are swapped, especially in the case of RGB, the resulting input will consist of “valid” color levels for all eight bars, but the order will be incorrect.*

How Results are Calculated First the bars are identified using the relative amplitudes of the three channels and the specification for the selected format and colorimetry.

The amplitudes are calculated using waveform averaged values within each identified bar relative to back porch. Thus, it is important to ensure that the sync signal is within the captured data window for valid measurements. For example, if a manual set-up is performed, not only are all eight bars required on the waveform display, but the entire horizontal blanking area to the right of the signal being measured is also required in order to locate the sync signal and the associated back porch.

Measuring Multiburst

The Multiburst measurement is used to verify frequencies and corresponding amplitudes of sinusoidal bursts. It can be used to verify the proper reconstruction of a band-limited video signal across the frequency spectrum. For example, a frequency roll-off (decrease in amplitude with increasing frequency) is seen with video from an analog-to-digital converter that lacks a reconstruction filter with $\sin(x)/x$ correction. In this example, quality is reduced by things like loss of detail in the video or color shifts in details.

Deviations in frequency from the reference test signal frequency (for example, a 30 MHz burst is rendered as a 20 MHz burst) may indicate things such as format change through frequency shift, frequency aliasing due to digital and/or analog re-sampling, and/or frequency aliasing due to the lack of a proper reconstruction filter.

The flag amplitude measurement can be used to verify the channel gain across a wider frequency range than each burst. Burst amplitudes are measured relative to the flag amplitude.

Signal Source

You can use the matrix signal, or you can use any multiburst signal with a reference flag preceding the bursts. The more cycles present in each burst, the more robust and generally more accurate the measurement will be. A burst with less than 2 cycles is not recommended.

The frequencies are always displayed from lowest to highest regardless of the order of burst frequencies in the multiburst signal. To avoid confusion regarding the correspondence between the results burst numbering and the signal burst ordering, a signal with increasing burst frequencies (from left to right) is recommended.

Interpreting Results

For multiburst signals free of non-linear distortion and with increasing burst frequencies, the “Frq(MHz)” column displays the fundamental frequency of burst specified in each row. The “Amp(dB)” column has the magnitude of the corresponding burst.

However, if non-linear distortion is present, interpreting results may be less straight forward.

In many consumer set-top boxes, lack of a reconstruction filter (with out-of-band rejection plus $\sin(x)/x$ correction) leads to roll-off in the fundamental frequency component of the bursts even though the envelope of the bursts may be flat on average. In this case, the amplitude results for the highest frequency may be low by a few dB even though the waveform shows the same burst with peak-to-peak amplitude closer to 0 dB. This indicates that the burst is no longer a pure windowed sinusoid, but has other spectral content (at least one alias frequency in

this example). If the extra spectral content is removed by filtering, the resulting sinusoid will have the amplitude shown in the results.

Generally, if the signal has undergone processing without a required anti-alias filter (as in re-sampling for format conversion, or signal reconstruction), each burst may contain one or several frequency aliases. In such cases, burst frequencies that increase with each burst of the input signal may contain burst frequencies in nearly any order in the output of the device under test.

For example, in the 480p rendering of an ATSC 1080i multiburst signal, 5 MHz is rescaled to 4.85 MHz, 10 MHz to 9.71, but 15 MHz, 20 MHz, 25 MHz, and 30 MHz become any number of frequencies (including 12.44 MHz, 7.58 MHz, 2.73 MHz, and 2.12 MHz respectively). These frequency aliases and respective amplitudes are measured and displayed in order: 2.12 MHz, 2.73 MHz, 4.85 MHz, 7.58 MHz, 9.71 MHz, 12.44 MHz.

How Results are Calculated

The six largest peaks are found in the spectrum of signal on the pedestal. These frequencies are displayed in order from lowest to highest. For each of these frequencies, the maximum magnitude of the cross-correlation between the signal within the pedestal area and a windowed complex sinusoid is found. This gives the amplitude.

Measuring Noise

The unweighted noise within the nominal bandwidth of the video signal is measured to ensure that the video quality is not reduced by random errors such as those that cause “snow.”

Signal Source You can use the matrix signal, or you can use any flat line or line pedestal signal.

Interpreting Results As a rule of thumb, errors generally become visible when the signal-to-noise dB measurement ranges in the low 40s. However, the degree of visibility depends on many factors, including spectral distribution of the noise. In standard definition television, noise weighting filters such as CCIR Recommendation (Rec) 576-2 unified weighting filter are used to weight the noise spectrum to better match the visibility of noise in typical viewing conditions. The unified weighting filter has been modified to exactly match the “visibility of noise characteristics” of 576-2 on the screen for each selected video format.

How Results are Calculated After line tilt and other low frequency distortions are removed from the signal, all AC signal content is spectrally weighted by the selected filter, if any, and the resulting RMS voltage is calculated along with the signal-to-noise ratio in dB using a 700mV peak signal value.

Measuring Non Linearity

This measurement is used to measure deviations from a straight line ramp test signal. Deviations can be caused by such things as soft-limiting from analog amplifiers and digital processing errors. Problems in linearity can reduce video quality by, for example, reducing contrast at various average luminance levels, creating color shifts.

Signal Source You can use the matrix signal, or you can use either a ramp or step signal. However, a ramp signal will give the best accuracy.

Interpreting Results The measurement shows deviations from linear increase in the test signal as a percentage of the largest increase per time found.

How Results are Calculated In the case of steps, results are deviations in step amplitudes in the test signal as a percentage of the largest step found.

In the case of ramps, using six equal time intervals across the ramp, results are deviations from linear increase in the test signal as a percentage of the largest increase per time found.

Measuring Sync

This measurement is used to check synchronization signal timing and amplitude, including the relative position of the start and end of active video (interpreted by looking at front and back porch times).

Signal Source You can use the matrix signal, or you can use a signal with signal amplitude greater than 7.5% at the beginning and end of active video in order to measure front porch and back porch times.

Interpreting Results The amplitudes are measured relative to back porch.
Selecting either 1080 or 720 formats will display the tri-level sync results.
Selecting either 480, 576, or SXGA will display the bi-level sync results.

How Results are Calculated The amplitudes are measured relative to back porch.
The times are taken as the time between half amplitudes of adjacent transitions. For example, “Neg. Sync Width” is the measured time between the half amplitude of the falling or leading edge of negative sync and the half amplitude of the rising or trailing edge of negative sync.
In the absence of sufficiently large (greater than 7.5%) video signal, the width of front porch and back porch may not be found. In this case, the measurement of the respective porch widths will not be valid.



Appendices

Appendix A: Specifications

All specifications are guaranteed unless labeled “typical.” Typical specifications are provided for your convenience but are not guaranteed. To meet specifications, the following conditions must be met:

- The oscilloscope must have been calibrated in an ambient temperature between 20 °C and 30 °C (68 °F and 86 °F).
- The oscilloscope must be operating within the environmental limits listed in Table A-10 on page A-16.
- The oscilloscope must be powered from a source that meets the specifications listed in Table A-8 on page A-15.
- The oscilloscope must have been operating continuously for at least 20 minutes within the specified operating temperature range.
- You must perform the Signal Path Compensation procedure after the 20-minute warm-up period. If the ambient temperature changes more than 5 °C (9 °F) you must restart the procedure. See *Signal Path Compensation* in the *Getting Started* chapter of the *TDS5000B Series Quick Start User Manual*.

Table A- 1: Video measurement specifications

Characteristic	Description	
Color bar measurement accuracy	± 2.0 mV ± 1.5 V% of reading	Measurement of all 8 bar levels, displayed in absolute (mV) values. YPbPr or RGB formats.
Noise measurement	<i>Range and Accuracy</i>	
Unweighted	-20 to -60 dB, ± 1 dB (30 MHz measurement bandwidth)	Noise measurement bandwidth selectable, 200 KHz to 250 MHz. Trigger on CH 4 required for measurements below -60 dB (30 MHz BW).
	-60 to -70 dB, ± 2 dB (30 MHz measurement bandwidth)	
Weighted	-20 to -60 dB, ± 2 dB	Unified Weighting Filter. Trigger on CH 4 required for measurements below -60 dB.
Noise floor	Less than -76 dB, 30 MHz noise bandwidth	Typical is less than -80 dB, 30 MHz noise bandwidth

Table A-1: Video measurement specifications (Cont.)

Characteristic	Description	
Multiburst measurement	<i>Accuracy</i>	
Flag amplitude	$\pm 2\text{mV} \pm 1.5\%$ of reading	
1 MHz to 10 MHz packets	± 0.5 dB	Measurement relative to reference flag amplitude
10 MHz to 30 MHz packets	± 0.75 dB	
Frequency readout		Multiburst packet frequency is measured and displayed.
Non-linearity measurement accuracy	1.5%	Non-linearity measurement using a ramp test signal. Incremental linearity reported over five equally spaced intervals, as well as an overall linearity figure for each channel.
Sync measurement	<i>Accuracy</i>	
Sync amplitude	$\pm 2\text{mV} \pm 1.5\%$ of reading	Blanking interval measurements, including sync amplitude, width, and rise time.
Sync timing	± 5 ns	
Rise and Fall time	± 5 ns	
Channel delay	CH 1 to CH 2, CH 1 to CH 3, CH 2 to CH 3; readouts in ns.	
	<i>Range</i>	<i>Accuracy</i>
Measurement	± 35 ns	± 5 ns
Delay match error	Less than 1 ns	Any two channels

Table A-2: Channel input and vertical specifications

Characteristic	Description
Input coupling	AC, DC, and GND
Input channels	Four identical channels
Input impedance selection	50 Ω or 1 M Ω Bandwidth limited to 500 MHz, 1 M Ω selected
Input impedance, DC coupled	50 Ω $\pm 2.5\%$, typical 1 M Ω $\pm 1.0\%$ in parallel with 18 pF ± 2 pF VSWR $\leq 1.5:1$, typical, from DC to 1 GHz
Maximum voltage at input BNC	AC, DC, or GND coupled

Table A-2: Channel input and vertical specifications (Cont.)

Characteristic	Description	
1 M Ω	150 V _{RMS} CAT I, and ≤ 400 peak For steady state sinusoidal waveforms, derate at 20 dB/decade above 200 kHz to 9 V _{RMS} at ≥ 3 MHz	
50 Ω	< 1 V _{rms} for settings below 100mV/div < 5 V _{rms} for 100 mV/div settings and above	
Differential delay, DC 50 Ω input	≤ 100 ps between any two channels with DC input coupling and the same V/div scale settings at or above 10 mV/div	
Deskew range, typical	± 75.0 ns	
Channel-to-channel crosstalk	$\geq 100:1$ at ≤ 100 MHz $\geq 30:1$ at > 100 MHz up to the rated bandwidth for any two channels with equal V/div settings	
Digitizers	8-bit resolution Four separate digitizers, each channel sampled simultaneously	
Sensitivity range	Fine adjustment available with $\leq 1\%$ resolution	
1 M Ω	1 mV/div to 10 V/div, in a 1-2-5 sequence	
50 Ω	1 mV/div to 1 V/div, in a 1-2-5 sequence	
Analog bandwidth	<i>SCALE range</i>	<i>Bandwidth</i>
	1 mV/div to 1.99 mV/div	DC to 175 MHz
	2 mV/div to 1 V/div	DC to 1 GHz
	DC 50 Ω coupling; bandwidth limit set to Full; operating ambient ≤ 30 °C; derated by 5 MHz/°C above 30 °C	
Analog bandwidth selections	20 MHz, 150 MHz, or Full	

Table A-2: Channel input and vertical specifications (Cont.)

Characteristic	Description		
Analog Bandwidth Limit			
Low frequency, AC coupled	50 Ω : < 200 kHz		
	1 M Ω : < 10 Hz, reduced by a factor of ten when using a 10X probe		
High frequency, typical	20 MHz: with 20 MHz bandwidth limit turned on		
	150 MHz: with 150 MHz bandwidth limit turned on		
Calculated rise time, typical	DC 50 Ω coupling, bandwidth limit set to Full		
	<i>SCALE range</i>	<i>Rise time</i>	
	1 mV/div to 1.99 mV/div	2.29 ns	
	2 mV/div to 1 V/div	300 ps	
Step response settling errors, typical	Bandwidth limit set to Full		
	<i>SCALE range</i>	<i>Settling error at time after step</i>	
	≤ 2 V step amplitude	1 mV/div to 99.5 mV/div	20 ns: $\leq 0.5\%$
			100 ns: $\leq 0.2\%$
			20 ms: $\leq 0.1\%$
	≤ 20 V step amplitude	100 mV/div to 1.0 V/div	20 ns: $\leq 1.0\%$
			100 ns: $\leq 0.5\%$
			20 ms: $\leq 0.2\%$
	≤ 200 V step amplitude	1.01 V/div to 10 V/div	20 ns: $\leq 1.0\%$
			100 ns: $\leq 0.5\%$
20 ms: $\leq 0.2\%$			
Position range	± 5 divisions		
Peak Detect or Envelope Mode Pulse Response	Capture of single event pulses		
	<i>Number of channels</i>	<i>Minimum pulse width</i>	
	1 or 2	400 ps	
	3 or 4	800 ps	
Offset range	User-adjustable input offset voltages		
	1 M Ω coupling	<i>SCALE range</i>	
		1 mV/div to 99.5 mV/div	± 1 V
		100 mV/div to 1 V/div	± 10 V
	1.01 V/div to 10 V/div	± 100 V	

Table A-2: Channel input and vertical specifications (Cont.)

Characteristic	Description	
50 Ω coupling	1 mV/div to 50 mV/div	± 0.5 V
	50.5 mV/div to 99.5 mV/div	± 0.25 V
	100 mV/div to 500 mV/div	± 5 V
	505 mV/div to 1 V/div	± 2.5 V
Offset accuracy	<i>SCALE range</i>	<i>Offset range</i>
	1 mV/div to 9.95 mV/div	$\pm[(0.2\% \times \text{net offset}) + 1.5 \text{ mV} + (0.1 \text{ div} \times \text{V/div setting})]$
	10 mV/div to 99.5 mV/div	$\pm[(0.35\% \times \text{net offset}) + 1.5 \text{ mV} + (0.1 \text{ div} \times \text{V/div setting})]$
	100 mV/div to 1.0 V/div	$\pm[(0.35\% \times \text{net offset}) + 15 \text{ mV} + (0.1 \text{ div} \times \text{V/div setting})]$
	1.01 V/div to 10 V/div	$\pm[(0.25\% \times \text{net offset}) + 150 \text{ mV} + (0.1 \text{ div} \times \text{V/div setting})]$
	Temperatures >40 °C	$\pm[(0.75\% \times \text{net offset}) + 150 \text{ mV} + (0.1 \text{ div} \times \text{V/div setting})]$
<i>where, net offset = offset - (position \times volts/division)</i>		

Table A-2: Channel input and vertical specifications (Cont.)

Characteristic	Description		
DC gain accuracy, Sample or Average acquisition mode	$\pm 3\% + 1.0\% \times \text{net offset /offset range} $ for 2 mV/div - 3.98 mV/div		
DC voltage measurement accuracy	<i>Measurement type</i>	<i>DC accuracy (in volts)</i>	
	Sample acquisition mode, typical	2 mV/div - 3.98 mV/div $\pm [(1.5\% + 3.0\% \times \text{net offset /offset range}) \times \text{reading} - \text{net offset} + \text{offset accuracy} + 0.13 \text{ div} \times \text{V/div setting} + 0.6 \text{ mV}]$	
	Delta voltage measurement between any two points acquired under the same setup and ambient conditions	2 mV/div - 3.98 mV/div $\pm [1.5\% + 3.0\% \times \text{net offset /offset range} \times \text{reading} - \text{net offset} + 0.26 \text{ div} \times \text{V/div setting} + 1.2 \text{ mV}]$	
	<i>Where, net offset = offset - (position \times volts/division)</i>		
✓ Average acquisition mode	Average of ≥ 16 waveforms	2 mV/div - 3.98 mV/div $\pm [1.5\% + 3.0\% \times \text{net offset /offset range} \times \text{reading} - \text{net offset} + \text{offset accuracy} + 0.06 \text{ div} \times \text{V/div}]$	
	Delta voltage measurement between any two averages of ≥ 16 waveforms acquired under the same setup and ambient conditions	2 mV/div - 3.98 mV/div $\pm [1.5\% + 3.0\% \times \text{net offset /offset range} \times \text{reading} - \text{net offset} + 0.1 \text{ div} \times \text{V/div} + 0.3 \text{ mV}]$	
	<i>Where, net offset = offset - (position \times volts/division)</i>		
Nonlinearity, typical	< 1 LSB differential, < 1 LSB integral, independently based		
Effective bits, typical	<i>Signal and input conditions</i>	<i>Signal and input conditions</i>	
	Sine wave input at the indicated frequency and pk-pk amplitude, 50 mV/div and 25 °C	1 MHz, 9.2 div, 5 GS/s sample rate, Sample acquisition mode	6.6 bits
		1 MHz, 9.2 div, 10 MS/s sample rate, HiRes acquisition mode	9.0 bits
		1 GHz, 6.5 div, 5 GS/s sample rate, Sample acquisition mode	4.7 bits

Table A-3: Horizontal and acquisition system specifications

Characteristic	Description	
Acquisition modes	Sample, Peak detect, Hi Res, Average, and Envelope	
Fast acquisition rate	Up to 100,000 waveforms-per-second with Fast Acquisition mode on	
	Up to 130 waveforms-per-second with Fast Acquisition mode off	
Minimum record length	500 points	
Maximum record length	Depends on number of active channels and amount of memory installed	
Standard	2,000,000 points (3 or 4 channels) 4,000,000 points (2 channels) 8,000,000 points (1 channel)	
Option 3M installed	4,000,000 points (3 or 4 channels) 8,000,000 points (2 channels) 16,000,000 points (1 channel)	
Sample rate range, real-time	<i>Number acquired channels</i>	<i>Sample rate range</i>
	1	1.25 S/s to 5 GS/s
	2	1.25 S/s to 2.5 GS/s
	3 or 4	1.25 S/s to 1.25 GS/s
Equivalent-time sample rate or interpolated waveform rate range	2.5 GS/s to 250 GS/s Listed values depend on the number of channels in use, horizontal scale, and resolution settings. Equivalent-time acquisition can be enabled or disabled. When disabled, waveforms are interpolated at the fastest time base settings.	
Seconds/division range	(s/div x 10) to 1,000 s	
Horizontal delay range	16 ns to 250 s	
Long term sample rate and delay time accuracy	±15 ppm over any ≥1 ms interval	
RMS aperture uncertainty, typical	≤ [3 ps + (0.1 ppm × record duration)] for real-time or interpolated records with a duration ≥1 minute	

Table A-3: Horizontal and acquisition system specifications (Cont.)

Characteristic	Description	
Delta time measurement accuracy	For a single channel, with signal amplitude > 5 div, reference level set at 50%, interpolation set to sin(x)/x, volts/division set to ≥ 5 mV/div, with (displayed risetime)/(sample interval) ratio between 1.4 and 4, where sample interval = 1/(real-time sample rate)	
	<i>Conditions</i>	<i>Accuracy</i>
	Single shot signal, Sample, or Hi Res acquisition mode, Full bandwidth	$\pm (15 \text{ ppm} \times \text{reading} + 0.3 \text{ sample intervals})$
	Average acquisition mode, ≥ 100 averages, Full bandwidth	$\pm (15 \text{ ppm} \times \text{reading} + 20 \text{ ps})$

Table A-4: Trigger specifications

Characteristic	Description	
Auxiliary trigger input resistance, typical	$\geq 1.5 \text{ k}\Omega$	
Maximum trigger input voltage, typical	$\pm 20 \text{ V}$ (DC or peak AC)	
Edge trigger sensitivity, Main and Delayed trigger	<i>Trigger Source</i>	<i>Sensitivity</i>
	Any channel, DC coupled	0.35 div from DC to 50 MHz, increasing to 1 div at 1 GHz
	Auxiliary input	400 mV from DC to 50 MHz, increasing to 750 mV at 100 MHz
Edge trigger sensitivity, typical	All sources, for vertical scale settings $\geq 10 \text{ mV/div}$ and $\leq 1 \text{ V/div}$	
	<i>Trigger coupling</i>	<i>Sensitivity</i>
	NOISE REJ	$3 \times$ the DC-coupled limits
	AC	Same as DC-coupled limits for frequencies $\geq 60 \text{ Hz}$; attenuates signals $< 60 \text{ Hz}$
	HF REJ	$1.5 \times$ the DC-coupled limits from DC to 30 kHz; attenuates signals $> 30 \text{ kHz}$

Table A- 4: Trigger specifications (Cont.)

Characteristic	Description	
	LF REJ	1.5 × the DC-coupled limits for frequencies ≥80 kHz; attenuates signals <80 kHz
Advanced trigger sensitivity, typical	For all trigger types except Edge, with vertical scale settings ≥10 mV/div and ≤1 V/div	
	1.0 div from DC to 500 MHz	
Event count sensitivity, typical	For sequential trigger delayed by events, with vertical scale settings ≥10 mV/div and ≤1 V/div	
	1.0 div, from DC to 500 MHz	
Video trigger sensitivity, typical	For delayed and main triggers, with vertical scale settings ≥10 mV/div and ≤1 V/div	
	Any channel	0.6 to 2.5 divisions of video sync tip
Video Trigger Format	Triggers from negative sync composite video, field 1 or field 2 for interlaced systems, any field, specific line, or any line for interlaced or noninterlaced systems	
	Supported systems include NTSC, PAL, SECAM, and analog HDTV	
Trigger level or threshold range	<i>Trigger Source</i>	<i>Sensitivity</i>
	Any channel	±10 divisions from center of screen
	Auxiliary input	±8 V
	Line	Fixed at zero volts

Table A-4: Trigger specifications (Cont.)

Characteristic	Description		
Trigger level or threshold accuracy, typical	Edge trigger, DC coupling, for signals having rise and fall times ≤ 20 ns		
	<i>Trigger Source</i>	<i>Accuracy</i>	
	Any channel	$\pm [(2\% \times \text{setting} - \text{net offset}) + (0.3 \text{ div} \times \text{volts/div setting}) + \text{offset accuracy}]$	
	Auxiliary	Not calibrated or specified	
	<i>Where, net offset = offset - (position \times volts/division)</i>		
Set level to 50% function, typical	Operates with signals ≥ 30 Hz		
Trigger position error, typical	Edge trigger, DC coupling, for signals having a slew rate at the trigger point of ≤ 0.5 div/ns		
	<i>Acquisition mode</i>	<i>Error</i>	
	Sample, Average	$\pm (1 \text{ displayed pt} + 1 \text{ ns})$	
	Envelope	$\pm (2 \text{ displayed pts} + 1 \text{ ns})$	
Trigger jitter, typical	$\sigma = 8$ ps RMS		
B Event (Delayed) trigger	<i>Trigger After Time</i>	<i>Trigger on n^{th} Event</i>	
	Range	Delay time = 16 ns to 250 s	
	Event count	1 to 10^7	
	Minimum time between arm (A Event) and trigger (B Event), typical	2 ns from the end of the time period to the B trigger event	
	Minimum time between the A trigger event and the first B trigger event	2 ns	
Minimum pulse width, typical	—	B event width ≥ 1 ns	
Maximum frequency, typical	—	B event frequency ≤ 500 MHz	
Advanced trigger timing	For vertical scale settings ≥ 10 mV/div and ≤ 1 V/div		
	<i>Minimum recognizable event width or time</i>	<i>Minimum rearm time to recognize next event</i>	
	Glitch type	Minimum glitch width = 1 ns	2 ns + 5% of glitch width setting
	Runt or window type	Minimum runt width = 2 ns	2 ns
	Runt or window type (time qualified)	Minimum runt width = 2 ns	8.5 ns + 5% of runt width setting
	Runt or window type (logic qualified)	Minimum runt width = 2 ns	8.5 ns + 5% of runt width setting

Table A- 4: Trigger specifications (Cont.)

Characteristic	Description	
Width type	Minimum difference between upper and lower limits = 1 ns	2 ns + 5% of upper limit setting
Timeout type	Minimum timeout time = 1 ns	2 ns + 5% of timeout setting
Transition type	Minimum transition time = 600 ps	8.5 ns + 5% of transition time setting
Pattern type, typical	Minimum time the pattern is true = 1 ns	1 ns
Logic	Not applicable	1 ns
Events Delay	1 ns (single channel)	Not applicable
State type, typical	Minimum true time before clock edge = 1 ns Minimum true time after clock edge = 1 ns	1 ns
Setup/Hold type, typical	<i>Minimum clock pulse width from active edge to inactive edge</i>	<i>Minimum clock pulse width from inactive edge to active edge</i>
	3 ns + hold time setting	2 ns
	<i>Setup and Hold parameters</i>	<i>Limits</i>
	Setup time (time from data transition to clock edge)	-100 ns minimum +100 ns maximum
	Hold time (time from clock edge to data transition)	-1 ns minimum +102 ns maximum
	Setup time + Hold time (algebraic sum of the two settings)	+2 ns minimum +202 ns maximum

Table A-4: Trigger specifications (Cont.)

Characteristic	Description	
Advanced trigger timer ranges	<i>Limits</i>	
Glitch type	1 ns to 1 s	
Runt or window type, wider than	1 ns to 1 s	
Runt or window type, time qualified	1 ns to 1 s	
Width type	1 ns to 1 s	
Timeout type	1 ns to 1 s	
Transition type	1 ns to 1 s	
Pattern type	1 ns to 1 s	
Setup/Hold type	<i>Setup and Hold timers</i>	<i>Limits</i>
	Setup time (time from data transition to clock edge)	-100 ns to +100 ns
	Hold time (time from clock edge to data transition)	-1 ns to +100 ns
	Setup time + Hold time (algebraic sum of the two settings)	+2 ns to +200 ns
Advanced trigger timer accuracy	For Glitch, Timeout, or Width types	
	<i>Time range</i>	<i>Accuracy</i>
	1 ns to 500 ns	±(20% of setting + 0.5 ns)
	520 ns to 1 s	±(0.01% of setting + 100 ns)
Trigger holdoff range	1.5 μ s to 12 s, minimum resolution is 8 μ s for settings \leq 1.2 ms	

Table A-5: Display specifications

Characteristic	Description
Display type	264 mm (10.4 in) diagonal, liquid crystal active-matrix color display Width: 211.2 mm (8.3 in) Length: 158.4 mm (6.2 in)
Display resolution	640 horizontal × 480 vertical pixels
Pixel pitch	0.33 mm horizontal, 0.33 mm vertical
Contrast ratio, typical	150:1
Response time, typical	50 ms, black to white
Display refresh rate	59.94 frames per second
Displayed intensity levels	Supports Windows SVGA high-color mode (16-bit or 24-bit)

Table A-6: Input/output port specifications

Characteristic	Description
Probe Compensator Output	Front-panel terminals <i>Output voltage</i> <i>Frequency</i> 1.0 V (from base to top) ±1.0% into a ≥ 10 kΩ load 1 kHz ±5%
Analog Signal Output	Rear-panel BNC connector, provides a buffered version of the signal that is attached to the channel 3 signal input 50 mV/div ±20% into a 1 MΩ load 25 mV/div ±20% into a 50 Ω load
Bandwidth, typical	100 MHz into a 50 Ω load
Auxiliary Output levels	Rear-panel BNC connector, provides a TTL-compatible, negative-polarity pulse for each A or B trigger (selectable) <i>V_{out high}</i> <i>V_{out low (true)}</i> ≥2.5 V into open circuit, ≥1.0 V into 50 Ω load ≤0.7 V with ≤4 mA sink, ≤0.25 V into 50 Ω load
Auxiliary Output pulse width, typical	Pulse width varies, 1 μs minimum
External Reference Input	Rear-panel BNC connector 9.8 MHz to 10.2 MHz 200 mV _{p-p} to 7 V _{p-p} < 1.5 kΩ in series with ~10 nF DC blocking capacitor
Side-panel I/O ports	Ports located on the side panel

Table A-6: Input/output port specifications (Cont.)

Characteristic	Description
Parallel port (IEEE 1284)	DB-25 connector, supports the following modes: Standard, output only Bidirectional, PS-2 compatible Bidirectional Enhanced Parallel Port (IEEE 1284 standard, mode 1 or mode 2, v 1.7) Bidirectional High-speed Extended Capabilities Port
Audio ports	Miniature phone jacks for stereo microphone input and stereo line output
USB port (2)	Allows connection of USB keyboard/mouse and or other devices while scope power is on Supports USB 2.0 protocol
Keyboard port	PS-2 compatible, oscilloscope power must be off to make connection
Mouse port	PS-2 compatible, oscilloscope power must be off to make connection
LAN port	RJ-45 connector, supports 10 base-T and 100 base-T
Serial port (COM1)	DB-9 connector, uses NS16C550-compatible UARTS, transfer speeds up to 115.2 kb/s
SVGA video port	Upper video port, DB-15 female connector, connect a second monitor to use dual-monitor display mode, supports Basic requirements of PC99 specifications
GPIB port	IEEE 488.2 standard interface
Scope VGA video port	Lower video port, DB-15 female connector, 31.6 kHz sync, EIA RS-343A compliant, connect to show the oscilloscope display, including live waveforms, on an external monitor

Table A-7: Data storage specifications

Characteristic	Description
CD-ROM	Side-panel CD-R/W drive; reads CD/CD-ROM, CD-R, and CD-R/W disks 24X read speed; 24X write speed
Floppy disk	Front-panel 3.5 in USB floppy disk drive, 1.44 MB capacity
Hard disk	Standard internal hard disk capacity: 80 GB External hard disk capacity: refer to added options

Table A- 8: Power source specifications

Characteristic	Description
Source voltage and frequency	100 to 240 V _{RMS} ±10%, 47 Hz to 63 Hz
Power consumption	≤ 220 Watts
Fuse rating	Internal to power supply; not serviceable by user
Nonvolatile memory retention	CMOS settings stored for a period of 3 years without instrument connection to power mains Calibration settings and error log entries stored for 1 million cycles or 20 years
Overvoltage Category	Overvoltage Category II (as defined in IEC61010-1/A2)

Table A- 9: Mechanical specifications

Characteristic	Description												
Weight													
Benchtop configuration	24.75 lbs (10.2 kg) oscilloscope only 56.5 lbs (25.6 kg) when packaged for domestic shipment												
Rackmount kit	5 lbs (2.3 kg) rackmount conversion kit 8 lbs (3.6 kg) kit packaged for domestic shipment												
Dimensions													
Benchtop configuration	Height: 14.2 in (360.7 mm) Height:, feet extended:14.25 in (362 mm) Width: 17.6 in (447 mm) Depth: 11.35 in (288.3 mm)												
Rackmount configuration (Option 1R)	Height: 10.5 in (267 mm) Width: 19 in (483 mm) Depth: 9.1 in (231 mm)												
Cooling	Fan-forced air circulation with no air filter												
Required clearances	<table border="1"> <tbody> <tr> <td>Top</td> <td>0 in (0 mm)</td> </tr> <tr> <td>Bottom</td> <td>0.25 in minimum or 0 in (0 mm) when standing on the feet</td> </tr> <tr> <td>Left side</td> <td>3 in (76 mm)</td> </tr> <tr> <td>Right side</td> <td>0 in [5 in (126 mm) required to access CD-ROM]</td> </tr> <tr> <td>Front</td> <td>0 in (0 mm)</td> </tr> <tr> <td>Rear</td> <td>0 in (0 mm)</td> </tr> </tbody> </table>	Top	0 in (0 mm)	Bottom	0.25 in minimum or 0 in (0 mm) when standing on the feet	Left side	3 in (76 mm)	Right side	0 in [5 in (126 mm) required to access CD-ROM]	Front	0 in (0 mm)	Rear	0 in (0 mm)
Top	0 in (0 mm)												
Bottom	0.25 in minimum or 0 in (0 mm) when standing on the feet												
Left side	3 in (76 mm)												
Right side	0 in [5 in (126 mm) required to access CD-ROM]												
Front	0 in (0 mm)												
Rear	0 in (0 mm)												

Table A-9: Mechanical specifications (Cont.)

Characteristic	Description
Construction material	Chassis parts constructed of aluminum alloy; front-panel constructed of plastic laminate; circuit boards constructed of glass laminate; outer shell molded and textured from a polycarbonate/ABS blend

Table A-10: Environmental specifications

Characteristic	Description
Temperature	
Operating	+5 °C to +45 °C (+41 °F to +113 °F)
Nonoperating	-20 °C to +60 °C (-4 °F to +140 °F)
Humidity	
Operating	20% to 80% relative humidity with a maximum wet bulb temperature of +29 °C (84.2 °F) at or below +45 °C (113 °F), noncondensing Upper limit derated to 30% relative humidity at +45 °C (113 °F)
Nonoperating	With no diskette in floppy disk drive 5% to 90% relative humidity with a maximum wet bulb temperature of +29 °C (84.2 °F) at or below +60 °C (+140 °F), noncondensing Upper limit derated to 20% relative humidity at +60 °C (+140 °F)
Altitude	
Operating	10,000 ft (3,048 m)
Nonoperating	40,000 ft (12, 190 m)
Random vibration	
Operating	0.1 g _R MimesS from 5 Hz to 500 Hz, 10 minutes on each axis
Nonoperating	2.0 g _{RMS} from 5 Hz to 500 Hz, 10 minutes on each axis
Shock, nonoperating	30 g (11 ms half-sine wave) or less

Table A- 11: Certifications and compliances

Category	Standards or description
EC Declaration of Conformity - EMC	<p>Meets intent of Directive 89/336/EEC for Electromagnetic Compatibility. Compliance was demonstrated to the following specifications as listed in the Official Journal of the European Union:</p> <p>EN 61326 Emissions ^{1, 3, 4} Class A Radiated and Conducted Emissions</p> <p>EN 61326 Immunity ^{1, 4}</p> <p>IEC 61000-4-2 Electrostatic Discharge Immunity ±4 kV contact discharge, ±8 kV air discharge</p> <p>IEC 61000-4-3 RF field immunity 3 V/m, 80 MHz to 1 GHz, 80% amplitude modulated with a 1 kHz sinewave ²</p> <p>IEC 61000-4-4 Electrical Fast Transient/Burst Immunity 1 kV on AC mains, 500 V on I/O</p> <p>IEC 61000-4-5 AC Surge Immunity 500 V differential mode, 1 kV common mode</p> <p>IEC 61000-4-6 RF Conducted Immunity 3 V, 150 kHz to 80 MHz, amplitude modulated with a 1 kHz sinewave ²</p> <p>IEC 61000-4-11 AC Mains Voltage Dips and Interruption Immunity 100% reduction for one cycle</p> <p>EN 61000-3-2 Power Harmonic Current Emissions</p> <p>EN 61000-3-3 Voltage Changes, Fluctuations, and Flicker</p> <p>¹ Use low-EMI shielded interconnect cables, equivalent to the following Tektronix cables: GPIB cable: 012-0991-01, 012-0991-02, or 012-0991-03. RS-232 cable: 012-1213-00 or CA part number 0294-9. Centronics Cable: 012-1214-00 or LCOM part number CTL3VGAMM-5 VGA Cable.</p> <p>² Under these conditions, the specifications are amended as follows: 1 mV/division to 1 V/division: ≤0.2 division waveform displacement or ≤0.4 division increase in peak-to-peak noise.</p> <p>³ Radiated emissions may exceed the levels specified in EN 61326 when this instrument is connected to a test object.</p> <p>⁴ Tested in accordance with EN 61326 Annex D.</p>
FCC	Radiated and conducted emissions do not exceed the levels specified in FCC47 CFR, Part 15, Subpart B, for Class A equipment.

Table A- 11: Certifications and compliances (cont.)

Category	Standards or description
EC Declaration of Conformity - Low Voltage	<p>Compliance was demonstrated to the following specification as listed in the Official Journal of the European Union:</p> <p>Low Voltage Directive 73/23/EEC, amended by 93/68/EEC</p> <p>EN 61010-1/A2:1995 Safety requirements for electrical equipment for measurement control and laboratory use.</p>
U.S. Nationally Recognized Testing Laboratory Listing	<p>UL3111-1, First Edition Standard for electrical measuring and test equipment.</p>
Canadian Certification	<p>CAN/CSA C22.2, No. 1010.1-92 Safety requirements for electrical equipment for measurement, control, and laboratory use.</p>
Additional Compliance	<p>IEC61010-1/A2 Safety requirements for electrical equipment for measurement, control, and laboratory use.</p>
Installation (Overvoltage) Category	<p>Terminals on this product may have different installation (overvoltage) category designations. The installation categories are:</p> <p>CAT III Distribution-level mains (usually permanently connected). Equipment at this level is typically in a fixed industrial location.</p> <p>CAT II Local-level mains (wall sockets). Equipment at this level includes appliances, portable tools, and similar products. Equipment is usually cord-connected.</p> <p>CAT I Secondary (signal level) or battery operated circuits of electronic equipment.</p>
Pollution Degree	<p>A measure of the contaminates that could occur in the environment around and within a product. Typically the internal environment inside a product is considered to be the same as the external. Products should be used only in the environment for which they are rated.</p> <p>Pollution Degree 2 Normally only dry, nonconductive pollution occurs. Occasionally a temporary conductivity that is caused by condensation must be expected. This location is a typical office/home environment. Temporary condensation occurs only when the product is out of service.</p>
Safety Certification Compliance	
Equipment Type	Test and measuring
Safety Class	Class 1 (as defined in IEC 61010-1/A2) - grounded product
Pollution Degree	<p>Pollution Degree 2 as defined in IEC 61010-1/A2</p> <p>Rated for indoor use only</p>

Appendix B: Performance Verification

This Performance Verification checks that the VM5000 Option HD meets its video measurement specifications (Table A-1 in Appendix A, Specifications).

Prerequisites

- The test signal generator and VM5000 Option HD instrument require a minimum 20 minute warm-up time before doing any performance verification tests.
- Perform the VM5000 Option HD instrument internal system diagnostics in the Utilities menu. The instrument must pass the diagnostics before you can verify performance.
- Perform the VM5000 Option HD instrument Signal Path Calibration (SPC) procedure. The instrument must pass the SPC before you can verify performance.

Required Equipment

Table B- 1: Required test equipment

Item number and description	Minimum requirements	Example	Purpose
HD CAV Television Test Signal generator (one required)		Tektronix TG700 with AWVG7 module	All tests
Digital Multimeter (one required)	5-1/2 digits, better than 0.1% DC accuracy 0-1 V	Fluke 8842A or Fluke model 45	AWVG7 signal output test
75 Ω BNC Cable (four required)	42 inches (106.68 cm) long	Tektronix part number 012-0074-00	All tests
75 Ω precision BNC terminations (four required)	0.025% Accuracy	Tektronix part number 011-0102-03	All tests
Connector, Dual-Banana (one required)	Female BNC-to-dual banana	Tektronix part number 103-0090-00	AWVG7 signal output test
Connector, BNC 'T' (four required)	Male BNC-to-dual female BNC	Tektronix part number 103-0030-00	All tests
Coupler, Dual-Input BNC 'T' cable assembly (one required)	Female BNC-to-dual male BNC	Tektronix part number 067-0525-02	Channel delay match test

VM5000 Option HD Tests

Determine the AWVG7 Signal Output Amplitude

This procedure determines the test signal generator output signal amplitude. You will need this value for calculating measurements. This procedure assumes you are using a Tektronix TG700 test signal generator with an AWVG7 module. If you are using a different test signal source, modify the steps according to your particular setup.

Equipment required	HD CAV Television Test Signal generator (Tektronix TG700 with AWVG7 module) Digital multimeter 75 Ω BNC Cable (1) 75 Ω precision BNC terminations (1) Connector, Dual-Banana (1) Connector, BNC 'T' (1)
Prerequisites	The test signal generator and multimeter must warm up for at least 20 minutes prior to doing this test.

NOTE. Make sure that the AWVG7 generator module and the multimeter have had a warm up period of at least 20 minutes.

1. Connect the digital multimeter to the test signal source. Refer to Figure B-1 while doing the following steps:
 - a. Connect one end of a 75 Ω BNC cable to the upper CH 1 connector on the AWVG7 generator module.
 - b. Connect the other cable end to the digital multimeter with a BNC 'T' connector, 75 Ω precision termination, and BNC female-to-dual banana adapter.

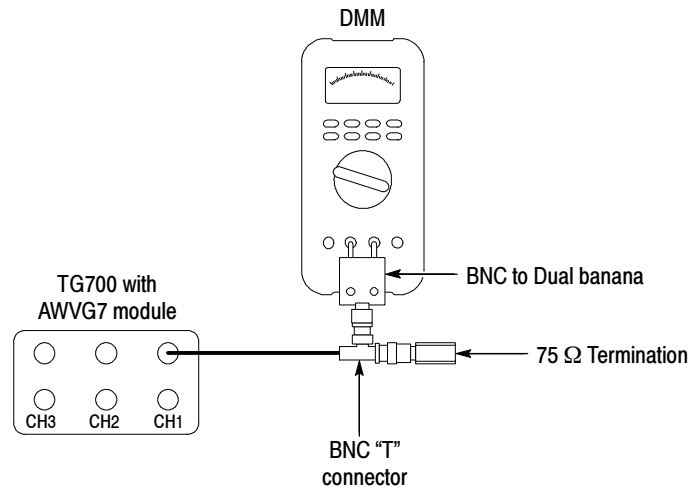


Figure B-1: Signal output amplitude test hookup

2. On the TG700, press the **MODULE**, **FORMAT**, and **FRONT PANEL ENABLE** buttons simultaneously, and then release the **MODULE** and **FORMAT** buttons. Continue to hold the **FRONT PANEL ENABLE** button to display **Factory Startup Mode**.
3. Enable the **DAC Gain (GBR) : 0 mV** calibration signal as follows:
 - a. Press the **MODULE** button to display the AWVG7 main menu.
 - b. Press the up or down arrow button to select **CALIBRATION**.
 - c. Press the left or right arrow button to select **DAC Gain (GBR)**.
 - d. Press the **ENTER** button.
 - e. Press the left or right arrow button to select **0 mV**.
 - f. Press the **ENTER** button.
4. Enter the digital multimeter reading in Table B-2, row DC0, column CH1.
5. Move the BNC cable from the upper CH 1 connector to the upper CH 2 connector on the AWVG7 generator module.
6. Enter the digital multimeter reading in Table B-2, row DC0, column CH 2.
7. Move the BNC cable from the upper CH 2 connector to the upper CH 3 connector on the AWVG7 generator module.
8. Enter the digital multimeter reading in Table B-2, row DC0, column CH 3.
9. On the TG700, press the left or right arrow button to select **700.397 mV**.

10. Press the ENTER button.
11. Enter the digital multimeter reading in Table B-2, row DC700, column CH 3.
12. Move the BNC cable from the upper CH 3 connector to the upper CH 2 connector on the AWVG7 generator module.
13. Enter the digital multimeter reading in Table B-2, row DC700, column CH 2.
14. Move the BNC cable from the upper CH 2 connector to the upper CH 1 connector on the AWVG7 generator module.
15. Enter the digital multimeter reading in Table B-2, row DC700, column CH 1.
16. Subtract the DC0 values from the DC700 values, for each of the three channels in Table B-2. The resulting three numbers are the Blanking-to-White levels for each channel.

Table B-2: Measured blanking to white levels

	CH 1	CH 2	CH 3
DC700 (measured)			
DC0 (measured)			
Blanking-to-white level (DC700 minus DC0)			

**Check Absolute
Amplitude Measurement
Accuracy**

This test verifies the measurement amplitude accuracy of the three video input channels (CH 1, CH 2, CH 3) and digitizers. This checks the accuracy specification for the Color Bars measurement, Multiburst Flag amplitude, and Sync Amplitude. The accuracy specification for all three is $\pm 2\text{mV} \pm 1.5\%$ of reading.

Equipment required	HD CAV Television Test Signal generator (Tektronix TG700 with AWVG7 module) 75 Ω BNC cables (4) 75 Ω precision BNC terminations (4) Connector, BNC 'T' (4)
Prerequisites	The test signal generator must warm up for at least 20 minutes prior to doing this test. You must have completed the procedure <i>Determine the AWVG7 Signal Outlet Amplitude</i> on page B-2.

1. Connect the instrument to the test signal source. Refer to Figure B-2 while doing the following steps:
 - a. Connect a 75 Ω BNC cables to each of the upper CH1, CH2, and CH3 AWVG7 outputs.
 - b. Connect the other end of each cable to a BNC 'T' connector and a precision 75 Ω termination.
 - c. Connect the BNC 'T' connector to the VM5000 Option HD, so that the cable from the AWVG7 CH1 output goes to the VM5000 Option HD CH1 input.
 - d. Connect the CH2 cable to the VM5000 Option HD CH2 input and the CH3 cable to the VM5000 Option HD CH3 input.

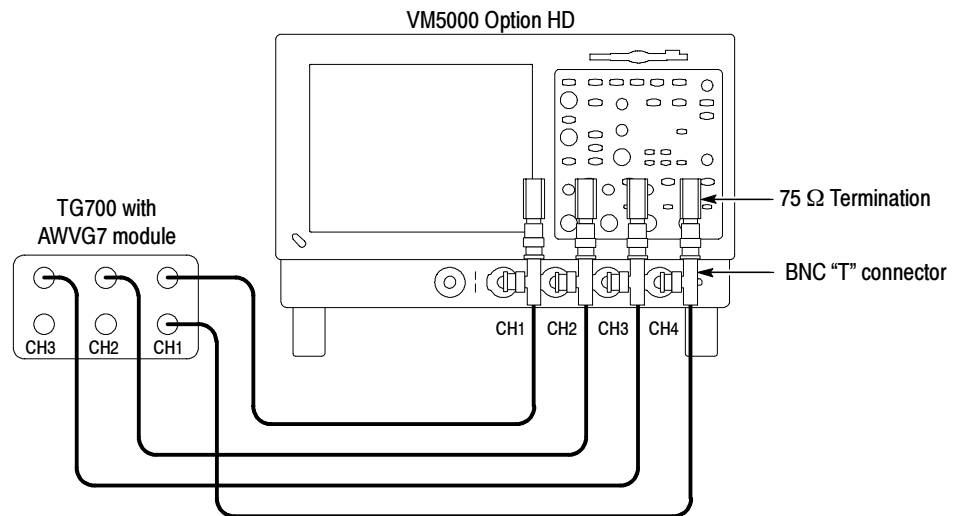


Figure B-2: Amplitude accuracy test hookup

- e. Connect a fourth 75 Ω BNC cable to the lower AWVG7 CH1 output.
 - f. Connect the other end of this cable to a BNC ‘T’ connector and a 75 Ω termination.
 - g. Connect the BNC ‘T’ connector to the VM5000 Option HD CH4 input.
2. On the TG700, press the **MODULE**, **FORMAT**, and **FRONT PANEL ENABLE** buttons simultaneously to return the generator to normal operating mode.
 3. After it is finished loading, press **MODULE** repeatedly to display **AWVG7**.
 4. Press **FORMAT** repeatedly to display **1080 59i GBR**.
 5. Press **ENTER**.

NOTE. Press and hold the **FRONT PANEL ENABLE** button to unlock the front panel.

6. Press **COLOR BAR** repeatedly to display **100% Color Bars**.
7. Start the VM5000 Option HD application (**File > Applications > VM5000HD**). Wait for the window to open after selecting VM5000HD.
8. Select **File > Recall Default**.
9. Select **Configuration > Format**, and select **RGB Color Space**.

10. Select **Configuration > Operation**, and select **Channel 4** as the trigger. Uncheck (turn off) **All Measurement Warnings**.
11. Select the VM5000HD **Run** button. The color bar measurement results table should appear with continuously updated measurements.
12. In the Color bar measurements window, change the **Averages** setting to **64**.
13. Record the VM5000HD measurement value for the white bar measurement, for each of the three channels, in row 4 of Table B-3.

Table B-3: White bar measurement

	CH 1 (Y/G)	CH 2 (Pb/B)	CH 3 (Pr/R)
AWVG7 Blanking-to-White level (DC700-DC0) (from Table B-2)			
Lower white limit value (equation 1)			
Upper white limit value (equation 2)			
White measurement			
Equation 1: Lower White limit value = (DC700-DC0) X (0.985) - 2 mV			
Equation 2: Upper White limit value = (DC700-DC0) X (1.015) + 2 mV			

14. Calculate the instrument white bar measurement as follows:
 - a. Copy the AWVG7 Blanking-to-White level values (from Table B-2, row 3) for each channel in row 1 of Table B-3.
 - b. For each channel, calculate the Lower VM5000HD white limit, using equation 1, and enter the values in row 2, Table B-3.
 - c. For each channel, calculate the Upper VM5000HD white limit, using equation 2, and enter the values in row 3, Table B-3.
15. Check that the VM5000HD white measurement (row 4) falls between the Lower (Line 2) and Upper (Line 3) limit values, for all three channels.

Table B-4 is an example of typical measurements and the calculation results.

Table B-4: Example white bar measurement values

	CH 1 (Y/G)	CH 2 (Pb/B)	CH 3 (Pr/R)
AWVG7 Blanking-to-White level (DC700-DC0) (from Table B-2)	700.05 mV	700.00 mV	701.04 mV
Lower white limit value (equation 1)	687.55 mV	687.50 mV	688.52 mV
Upper white limit value (equation 2)	712.55 mV	712.50 mV	713.56 mV
White measurement	696.55 mV	700.25 mV	695.01 mV
Equation 1: Lower White limit value = (DC700-DC0) X (0.985) - 2 mV			
Equation 2: Upper White limit value = (DC700-DC0) X (1.015) + 2 mV			

The calculated VM5000HD white measurements in row 4 are between the LOWER and UPPER limit values (rows 2 and 3), so the measurements are within specification for all channels.

Check Frequency Response Measurement Accuracy

This test verifies the frequency response accuracy of the three VM5000 Option HD video input channels (CH 1, CH 2, CH 3) and digitizers. This directly checks the Multiburst measurement accuracy, and indirectly the Noise measurement up through 30 MHz. The Multiburst accuracy specification is $\pm 0.5\text{dB}$ up through 10MHz, and $\pm 0.75\text{dB}$ from 10 to 30 MHz.

Equipment required	HD CAV Television Test Signal generator (Tektronix TG700 with AWVG7 module) 75 Ω BNC cables (4) 75 Ω precision BNC terminations (4) Connector, BNC 'T' (4)
Prerequisites	The test signal generator must warm up for at least 20 minutes prior to doing this test.

NOTE. The AWVG7 must meet its frequency response specification of $\pm 1\%$ (0.09dB) to 20 MHz, $\pm 2\%$ (0.17dB) to 28 MHz, and $\pm 3\%$ (0.26dB) to 30 MHz. If you are uncertain about the test signal generator calibration status, perform the AWVG7 frequency response performance verification described in the AWVG7 Service Manual.

1. Connect the instrument to the test signal source. Refer to Figure B-3 while doing the following steps:
 - a. Connect 75 Ω BNC cables to the upper CH1, CH2, and CH3 AWVG7 outputs.
 - b. Connect the other end of each cable to a BNC T connector and a 75 Ω termination.
 - c. Connect the BNC T connector to the VM5000 Option HD, so that the cable from the AWVG7 CH1 output goes to the VM5000 Option HD CH1 input.
 - d. Connect the CH2 cable to the VM5000 Option HD CH2 input and the CH3 cable to the VM5000 Option HD CH3 input.
 - e. Connect a fourth 75 Ω BNC cable to the lower AWVG7 CH1 output.
 - f. Connect the other end of this cable to a BNC T connector and a 75 Ω termination.
 - g. Connect the BNC T connector to the VM5000 Option HD CH4 input.

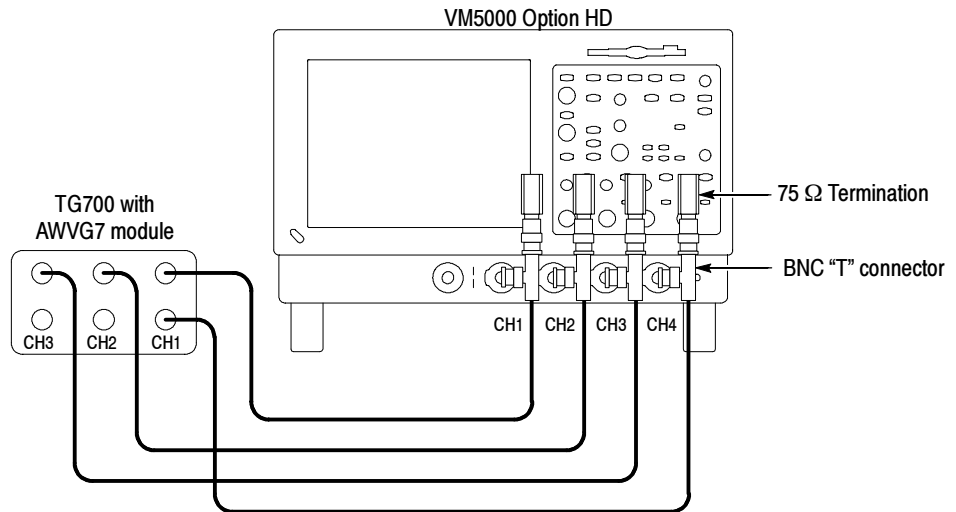


Figure B-3: Frequency accuracy test hookup

2. On the TG700, press **Module** repeatedly to display **AWVG7**.
3. Press **FORMAT** repeatedly to display **1080 59i GBR**.
4. Press **ENTER**.
5. Press **Multiburst** repeatedly to display **Multiburst 1-10 MHz**.

NOTE. Press and hold the **FRONT PANEL ENABLE** button to unlock the front panel.

6. Start the VM5000 Option HD application (**File > Applications > VM5000HD**).
7. Select **File > Recall Default**.
8. Select **Configuration > Format**.
9. Select **RGB Color Space**.
10. Select **Configuration > Measurements**.
11. Select the **Multiburst** check box and deselect the **Color Bars** check box.
12. Select **Configuration > Operation**, and select **Channel 4** as the trigger.
13. Select **Results > Multiburst**.

14. Select the VM5000HD **Run** button. The Multiburst measurement results table should display with continuously updated measurements.
15. Change the **Averages** setting to **64**.
16. Check the following:
 - a. The six Multiburst packet Amp(dB) readings (1, 2, 4, 6, 8, and 10 MHz) should be less than ± 0.5 dB, for each of the three channels (G, B, R).
 - b. The flag amplitude for each channel should be $420.0 \text{ mV} \pm 8.3 \text{ mV}$.
17. Select the VM5000HD **Stop** button to halt measurement.
18. Press the TG700 **Multiburst** button repeatedly to display **Multiburst 10-20 MHz**.
19. Select the VM5000HD **Run** button.
20. Check the following:
 - a. The six Multiburst packet Amp(dB) readings (10, 12, 14, 16, 18, and 20 MHz) should be less than ± 0.75 dB, for each of the three channels (G, B, R).
 - b. The flag amplitude for each channel should be $420.0 \text{ mV} \pm 8.3 \text{ mV}$.
21. Select the VM5000HD **Stop** button to halt measurement.
22. Press the TG700 **Multiburst** button repeatedly to display **Multiburst 20-30 MHz**.
23. Select the VM5000HD **Run** button.
24. Check the following:
 - a. The six Multiburst (20, 22, 24, 26, 28, and 30 MHz) packet Amp(dB) readings are less than ± 0.75 dB, for each of the three channels (G, B, R).
 - b. The flag amplitude for each channel should be $420.0 \text{ mV} \pm 8.3 \text{ mV}$.
25. Exit before the check that follows.

Check Noise Floor Measurement Accuracy

This test verifies the noise floor of the three VM5000 Option HD video input channels (CH 1, CH 2, CH 3) and digitizers. Noise floor affects the linearity of the noise measurement between -60 and -70 dB. The -76 dB Noise Floor specification ensures a noise floor error contribution of less than 1 dB for a -70 dB noise measurement. Together with the Amplitude Accuracy (Check A) and Frequency Response (Check B) checks, this indirectly checks the Noise measurement accuracy.

Equipment required	HD CAV Television Test Signal generator (Tektronix TG700 with AWVG7 module) 75 Ω BNC cable (1) 75 Ω precision BNC terminations (4) Connector, BNC 'T' (1)
Prerequisites	The test signal generator must warm up for at least 20 minutes prior to doing this test.

1. Connect the instrument to the test signal source. Refer to Figure B-4 while doing the following steps:
 - a. Connect a 75 Ω BNC cable to the CH1 AWVG7 outputs.
 - b. Connect the other end of the cable to the VM5000 Option HD CH 4 input and a 75 Ω termination using a BNC 'T' connector.
 - c. Place 75 Ω terminations on the VM5000 Option HD CH 1, CH 2, and CH 3 inputs.

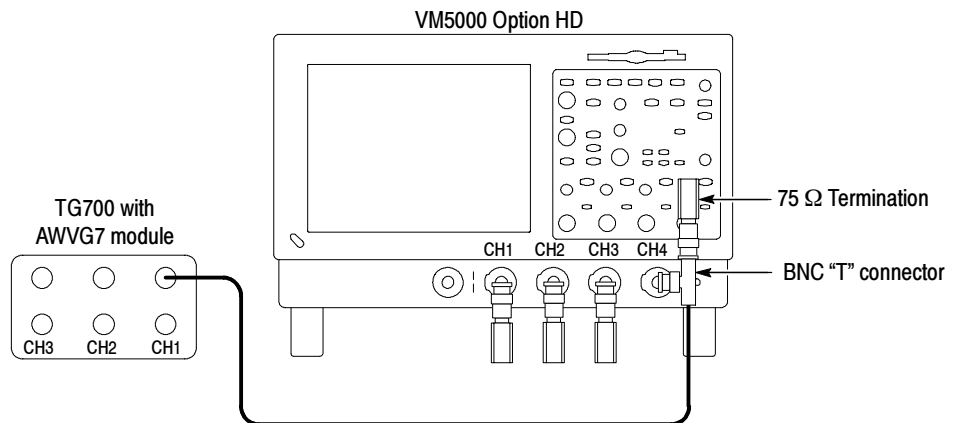


Figure B-4: Noise floor accuracy test hookup

2. Start the VM5000HD application (**File > Applications > VM5000HD**).
3. Select **File > Recall Default**.
4. Select **Configuration > Format** and select **RGB Color Space**.
5. Select **Configuration > Measurements**.
6. Select the **Noise** check box and deselect the **Color Bars** check box.

7. Select **Configuration > Operation**, and select **Channel 4** as the trigger.
8. Select **Results > Noise**.
9. Select **Unweighted BW** in the Filter area.
10. Adjust the **Bandwidth Hz** setting to **30.0 MHz**.
11. Change the **Averages** setting to **64**.
12. Select the VM5000HD **Run** button. The Noise measurement results table should appear with continuously updating measurements.
13. Check that the noise measurement dB values are greater than 76 dB for all three channels.

For example, a 78 dB reading passes. A 74 dB reading fails.

Check Channel Delay Match

This check verifies the delay match between the VM5000 Option HD CH 1, CH 2, and CH 3 measurement channels. Delay match error affects Channel Delay measurement accuracy. The specification for delay match error between any two channels is less than 1 ns.

Equipment required	HD CAV Television Test Signal generator (Tektronix TG700 with AWVG7 module) 75 Ω BNC cables (2) 75 Ω precision BNC terminations (2) Connector, BNC 'T' (2) Coupler, Dual-Input BNC 'T' cable assembly (1)
Prerequisites	The test signal generator must warm up for at least 20 minutes prior to doing this test.

1. Connect the instrument to the test signal source. Refer to Figure B-5 while doing the following steps:
 - a. Connect a 75 Ω BNC cable to the upper CH1 AWVG7 output.
 - b. Connect the other end of the cable to a BNC 'T' connector, BNC 'T' Cable Assembly, and 75 Ω termination.
 - c. Connect the BNC 'T' Cable Assembly to the VM5000 Option HD CH 1 and CH 2 inputs.
 - d. Connect a second 75 Ω BNC cable to the lower CH1 AWVG7 output.

- e. Connect the other end of the cable to the VM5000 Option HD CH 4 input and a 75 Ω termination using a BNC 'T' connector.

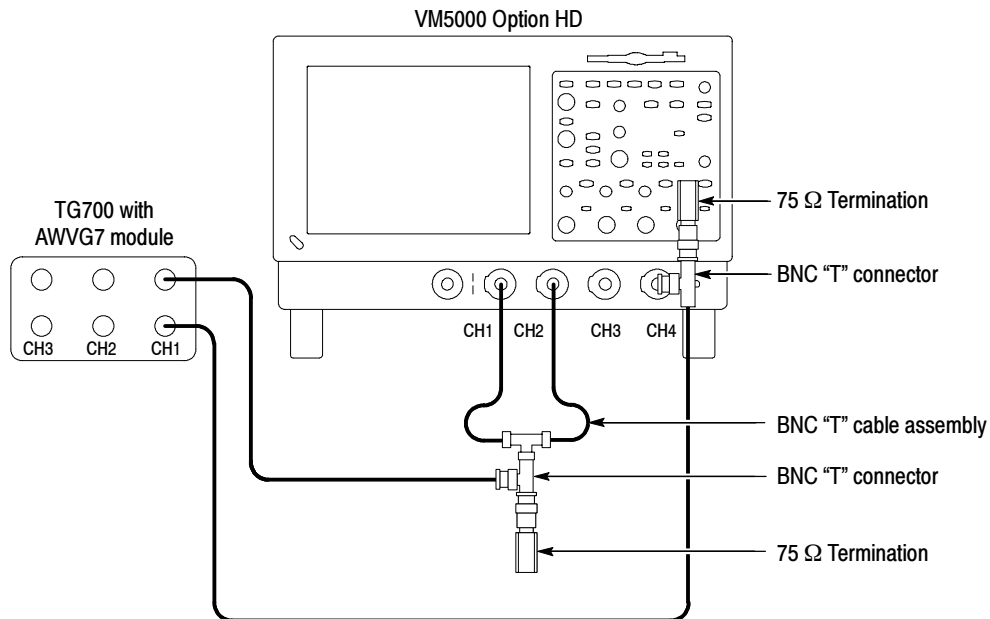


Figure B-5: Channel delay match test hookup

2. On the TG700, press the **Module** button repeatedly to display **AWVG7**.
3. Press **FORMAT** repeatedly to display **1080 59i GBR**.
4. Press **ENTER**.
5. Press **Multiburst** repeatedly to display **Multiburst 10-20 MHz**.

NOTE. Press and hold the **FRONT PANEL ENABLE** button to unlock the front panel.

6. Start the VM5000 Option HD application (**File > Applications > VM5000HD**).
7. Select **File > Recall Default**.
8. Select **Configuration > Format** and select **RGB Color Space**.
9. While still in **Configuration > Measurements**, select the **Channel Delay** check box and deselect the **Color Bars** check box.

10. Select **Configuration > Operation**:
 - a. Deselect all the **Warning Reporting** boxes.
 - b. Select **Channel 4** as the trigger.
11. Select **Results > Channel Delay**.
12. Change the **Averages** setting to **64**.
13. Select the VM5000HD **Run** button. The Channel Delay measurement results table should appear with continuously updating measurements.
14. Note the G-B measurement results (including sign) in row 1 of Table B-5.
15. Reverse the BNC ‘T’ Cable connections on CH 1 and CH 2.
16. Note the G-B measurement results (including sign) in row 2 of Table B-5.
17. Subtract line 2 from line 1 in Table B-5. Divide this result by 2 and enter it in row 3 of Table B-5.

Table B-5: Delay error measurements

	G-B (ns)	G-R (ns)	B-R (ns)
Connection 1			
Connection 2			
Net delay error (equation 3)			
Equation 3: [(Connection 1) - (Connection 2)] ÷ 2			

18. Connect the BNC ‘T’ Cable to the VM5000 Option HD CH 1 and CH 3 inputs. Repeat the procedure in steps 14 through 17 for the G-R measurement.
19. Connect the BNC ‘T’ Cable to the VM5000 Option HD CH 2 and CH 3 inputs. Repeat the procedure in steps 14 through 17 for the B-R measurement.
20. Check that the net delay error (row 3) is less than ±1 ns for G-B, G-R, and B-R.

This completes the VM5000 Option HD performance verification.

Appendix C: Remote Commands

You can control the VM5000 Option HD through the GPIB interface using commands and queries. The remote commands have the same functionalities as the menus and buttons in the user interface. You can see the effect of the commands on the interface as they are received.

NOTE. All oscilloscope platform GPIB commands are supported on the VM5000 Option HD instrument. For documentation on these commands, please refer to the TDS5000B GPIB Online Programmer Guide provided on the TDS5000B product software CD (Tektronix part number 063-3692-XX); see the installation instructions in the CD booklet.

This section covers the following information:

- *Syntax*, page C-1
- *Remote Startup and Exit of the Instrument*, page C-3
- *Command Groups*, page C-4
- *Commands*, on page C-8
- *Warning and Error Messages*, on page C-70

Syntax

Commands consist of set commands and query commands (usually simply called commands and queries). Commands modify the VM5000HD settings or tell the instrument to perform a specific action. Queries cause the VM5000 Option HD to return data and information about its status.

Most commands have both a set and a query form, although some commands only have a query form.

Command Structure

VM5000 Option HD instrument commands have the structure:

`:VARIABLE:VALUE "<Command>", "<Argument>"`

- You can abbreviate `VARIABLE:VALUE` to `VARIABLE:VAL` if desired, and it is case insensitive.
- There are no abbreviated versions of the `"<Command>", "<Argument>"` part of the VM5000 Option HD commands; you must enter the full name of this part of a command.

- The <Command> field is case sensitive, and use of incorrect command case spelling can result in unexpected results.
- All commands have a single <Argument>, which is case insensitive and cannot be the empty string "".
- Arguments are limited to a maximum of 60 characters. Arguments longer than 60 characters can cause unexpected behavior of the instrument and may require the application to be restarted, so this should be avoided.
- The comma character (,) and the double quote character (") are special characters and should not be used in the argument, otherwise unexpected behavior can result. All other printable characters are permitted in the argument.
- Commands that accept numeric arguments accept either integer or floating point values, with or without an exponent. This is equivalent to GPIB standard numeric formats <NR1>, <NR2>, and <NR3>.
- The VM5000 Option HD instrument does not support using a semicolon (;) to concatenate commands.

Query Structure

VM5000 Option HD instrument queries have the structure:

:VARIable:VALue? "<Command>"

- You can abbreviate VARIable:VALue? to VARI:VAL? if desired, and it is case insensitive.
- There are no abbreviated versions of the "<Command>" part of the VM5000 Option HD queries; you must enter the full name of a query.
- The <Command> field is case sensitive, and use of incorrect command case spelling can result in unexpected results.
- The VM5000 Option HD does not support using a semicolon (;) to concatenate queries.
- Query responses are always in upper case.
- The units and precision of result queries are identical to those in the user interface and those produced by generating a report.

Remote Startup and Exit of the Instrument

To start the application using remote commands, use the following command:

```
application:activate "VM5000HD"
```

To exit the application using remote commands, use the following command:

```
VARIABLE:VALUE "application", "exit"
```

You can check whether or not the VM5000 Option HD application is running using the following query:

```
VARIABLE:VALUE? "application"
```

If the application is running, this query will return "VM5000HD". However, if the application is not currently running, it will return the empty string "".

Command Groups

Tables C-1 through C-7 list the commands organized by functional group. (Refer to the Table of Contents for a list of all the commands in alphabetical order.)

Table C-1: Configuration commands

Header	Description
:VARIABLE:VALue	
AutoScale	Set or query whether to use auto scale during measurement
ChannelDelaySet	Set or query whether to measure channel delay upon Execute
ColorBarsSet	Set or query whether to measure Color Bars upon Execute
ColorSpace	Set or query the video color space to use for measurement
Format	Set or query the video format to use for measurement
MultiBurstSet	Set or query whether Multiburst is to be measured upon Execute
NoiseSet	Set or query whether Noise is to be measured upon Execute
NonLinearitySet	Set or query whether Non-Linearity is to be measured upon Execute
RunMode	Set or query run mode to use for measurement
SetupAndOrRun	Set or query setup mode to use for measurement
SyncSet	Set or query whether Sync is to be measured upon Execute
Trigger	Set or query the video trigger to use for measurement
WarningReportingMeasure	Set or query whether measurement warnings create a warning message
WarningReportingResults	Set or query whether results warnings are to create a warning message
WarningReportingSignal	Set or query whether signal warnings create a warning message

Table C-2: Miscellaneous commands

Header	Description
:VARIABLE:VALue	
Error	Reset error to 0 or query error value.
ID?	Query the ID/Version of the application
OPComplete	Controls VM5000 Option HD GPIB scripts by ensuring that the previous command is ready before either querying its value or calling the next command.
Warning	Reset warning to 0 or query warning value.

Table C- 3: Reports commands

Header	Description
:VARIABLE:VALue	
ReportGenerate	Generates a measurement report of the specified type (if a measure has been run and results are available), and saves it in the specified file
ReportMeasurements	Set or query the measurements to write to the report when ReportGenerate is called
ReportString	Set or query any additional information to write to the report when ReportGenerate is called

Table C- 4: Results commands

Header	Description
:VARIABLE:VALue:	
ChannelDelayAll?	Query all three delay measurements performed by Channel Delay
ChannelDelayCh1Ch2?	Query the Ch1Ch2 delay measurement performed by Channel Delay
ChannelDelayCh1Ch3?	Query the Ch1Ch3 delay measurement performed by Channel Delay
ChannelDelayCh2Ch3?	Query the Ch2Ch3 delay measurement performed by Channel Delay
ColorBarsmVCh[1..3]?	Query all eight level values resulting from Color Bars measurement for the specified channel
ColorBarsmVCh[1..3]Val[1..8]?	Query the value resulting from the specified Color Bars channel and value measurement
MultiburstAmpdBCh[1..3]?	Query all six amplitude values resulting from the specified Multiburst channel measurement
MultiburstAmpdBCh[1..3]Val[1..6]?	Query the amplitude value resulting from the specified Multiburst channel and value measurement
MultiburstFlagmVCh[1..3]?	Query the Flag value resulting from Multiburst measurement for the specified channel
MultiburstFreqCh[1..3]?	Query all six frequency values resulting from the specified Multiburst channel measurement
MultiburstFreqCh[1..3]Val[1..6]?	Query the frequency value resulting from the specified Multiburst channel and value measurement
NoiseAmpdBCh[1..3]?	Query amplitude value (in dB) resulting from Noise measurement for the specified channel
NoiseAmpmVCh[1..3]?	Query amplitude value (in mV) resulting from Noise measurement for the specified channel
NonLinearityPctCh[1..3]?	Query all six non-linearity values resulting from the Non-Linearity measurement for the specified channel

Table C-4: Results commands (Cont.)

Header	Description
NonLinearityPctCh[1..3]Max?	Query the maximum non-linearity value for the specified channel
NonLinearityPctCh[1..3]Val[1..5]?	Query the maximum non-linearity value for the specified channel and value
SyncLevelsMv?	Query all synchronization levels resulting from the Sync measurement
SyncLevelsMvVal[1..3]?	Query the specified synchronization level resulting from the Sync measurement
SyncTimes?	Query all synchronization times resulting from the Sync measurement
SyncTimesVal[1..7]?	Query the specified synchronization time resulting from the Sync measurement

Table C-5: Run commands

Header	Description
:VARIABLE:VALue	
Execute	Execute or stop the current set measurement(s), or query whether any measurement is currently being executed

Table C-6: Settings commands

Header	Description
:VARIABLE:VALue	
DefaultSettings	Restore default (factory) settings
RecallSettings	Recall settings stored in the specified path/filename
SaveSettings	Save current settings in the specified path/filename

Table C-7: Setup commands

Header	Description
:VARIABLE:VALue	
ChannelDelayAverage	Set or query the number of samples over which to average the Channel Delay measurement
ChannelDelayLine	Set or query line number that is to be used for the Channel Delay measurement
ColorBarsAverage	Set or query the number of samples over which to average the Color Bars measurement
ColorBarsLine	Set or query line number that is to be used for the Color Bars measurement

Table C- 7: Setup commands (Cont.)

Header	Description
MultiburstAverage	Set or query the number of samples over which to average the Multiburst measurement
MultiburstLine	Set or query line number that is to be used for the Multiburst measurement
NoiseAverage	Set or query the number of samples over which to average the Noise measurement
NoiseBW	Set or query bandwidth of noise filter that is to be used for Noise measurement, if the unweighted noise filter is selected
NoiseFilter	Set or query type of noise filter that is to be used for Noise measurement
NoiseLine	Set or query line number that is to be used for the Noise measurement
NonLinearityAverage	Set or query the number of samples over which to average the Non-Linearity measurement
NonLinearityLine	Set or query line number that is to be used for the Non-Linearity measurement
SyncAverage	Set or query the number of samples over which to average the Sync measurement
SyncLine	Set or query line number that is to be used for the Sync measurement

Commands

The following remote commands are listed in alphabetical order.

AutoScale < setting >

Set or query whether auto scale is to be used during measurement.

Syntax VARIable:VALue "AutoScale", "< setting >"
 VARIable:VALue? "AutoScale"

Group Configuration

Arguments < setting > specifies auto scale setting that is to be used.
 Valid settings are: OFF, ON, 0, 1.

Returns Query returns the current specified setting.

Examples VARIable:VALue "AutoScale", "ON"
 VARIable:VALue? "AutoScale"

Query may return: "AutoScale 0"

ChannelDelayAll?

Query all 3 delay measurements performed by Channel Delay.

Syntax VARIable:VALue? "ChannelDelayAll"

Group Results

Arguments None

Related Commands ChannelDelayCh1Ch2
ChannelDelayCh1Ch3
ChannelDelayCh2Ch3

Returns Returns all three delay measurements (in nanoseconds) performed by Channel Delay, in this order: Ch1Ch2 Ch1Ch3 Ch2Ch3.

Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "ChannelDelayAll"

Query may return: "ChannelDelayAll 1.84 0.04 -1.54"

ChannelDelayAverage < samples >

Set or query the number of samples over which to average the Channel Delay measurement.

Syntax VARIable:VALue "ChannelDelayAverage", "< samples >"
 VARIable:VALue? "ChannelDelayAverage"

Group Setup

Arguments < samples > can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current number of samples for Channel Delay measurement.

Examples VARIable:VALue "ChannelDelayAverage", "1"
 VARIable:VALue? "ChannelDelayAverage"

Query may return: "ChannelDelayAverage 8"

ChannelDelayCh1Ch2?

Query the Ch1Ch2 delay measurement performed by Channel Delay.

Syntax VARIable:VALue? "ChannelDelayCh1Ch2"

Group Results

Arguments None

Related Commands ChannelDelayAll
ChannelDelayCh1Ch3
ChannelDelayCh2Ch3

Returns Returns the Ch1Ch2 delay measurement (in nanoseconds) performed by Channel Delay.

Returns "---" if no valid measurement is currently available.

Examples VARIable:VALue? "ChannelDelayCh1Ch2"

Query may return: "ChannelDelayCh1Ch2 1.84"

ChannelDelayCh1Ch3?

Query the Ch1Ch3 delay measurement performed by Channel Delay.

Syntax VARIable:VALue? "ChannelDelayCh1Ch3"

Group Results

Arguments None

Related Commands ChannelDelayAll
 ChannelDelayCh1Ch2
 ChannelDelayCh2Ch3

Returns Returns the Ch1Ch3 delay measurement (in nanoseconds) performed by Channel Delay.

 Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "ChannelDelayCh1Ch3"

 Query may return: "ChannelDelayCh1Ch3 0.04"

ChannelDelayCh2Ch3?

Query the Ch2Ch3 delay measurement performed by Channel Delay.

Syntax VARIable:VALue? "ChannelDelayCh2Ch3"

Group Results

Arguments None

Related Commands ChannelDelayAll
ChannelDelayCh1Ch2
ChannelDelayCh1Ch3

Returns Returns the Ch2Ch3 delay measurement (in nanoseconds) performed by Channel Delay.

Returns "---" if no valid measurement is currently available.

Examples VARIable:VALue? "ChannelDelayCh2Ch3"

Query may return: "ChannelDelayCh2Ch3 -1.54"

ChannelDelayLine < linenumber >

Set or query line number that is to be used for Channel Delay measurement.

Syntax `VARIABLE:VALUE "ChannelDelayLine", "< linenumber >"`
`VARIABLE:VALUE? "ChannelDelayLine"`

Group Setup

Arguments `< linenumber >` can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current line number for Channel Delay measurement.

Examples `VARIABLE:VALUE "ChannelDelayLine", "200"`
`VARIABLE:VALUE? "ChannelDelayLine"`

Query may return: `"ChannelDelayLine 325"`

ChannelDelaySet < setting >

Set or query whether Channel Delay is to be measured upon Execute.

Syntax VARIable:VALue “ChannelDelaySet”, “< setting >”
 VARIable:VALue? “ChannelDelaySet”

Group Configuration

Arguments < setting > specifies whether to perform Channel Delay measurement upon Execute.
 Valid values are: OFF, ON, 0, 1.

Related Commands Execute
 ReportMeasurements

Returns Query returns 0 or 1 depending on whether ChannelDelaySet measurement is selected.

Examples VARIable:VALue “ChannelDelaySet”, “ON”
 VARIable:VALue? “ChannelDelaySet”
 Query may return: “ChannelDelaySet 1”

ColorBarsAverage < samples >

Set or query the number of samples over which to average the Color Bars measurement.

Syntax VARIable:VALue "ColorBarsAverage", "< samples >"
 VARIable:VALue? "ColorBarsAverage"

Group Setup

Arguments < samples > can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current number of samples for Color Bars measurement.

Examples VARIable:VALue "ColorBarsAverage", "1"
 VARIable:VALue? "ColorBarsAverage"

Query may return: "ColorBarsAverage 8"

ColorBarsLine < linewidth >

Set or query line number that is to be used for Color Bars measurement.

Syntax VARIable:VALue "ColorBarsLine", "< linewidth >"
 VARIable:VALue? "ColorBarsLine"

Group Setup

Arguments < linewidth > can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current line number for Color Bars measurement.

Examples VARIable:VALue "ColorBarsLine", "200"
 VARIable:VALue? "ColorBarsLine"

Query may return: "ColorBarsLine 325"

ColorBarsmVCh[1..3]?

Query all eight level values (in mV) resulting from the Color Bars measurement for the specified channel.

Syntax VARIable:VALue? "ColorBarsmVCh[1..3]"

Group Results

Arguments None

Related Commands ColorBarsmVCh[1..3]Val[1..8]

Returns Returns all eight delay measurements (in mV) performed by Color Bars, in this order: White Yellow Cyan Green Magenta Red Blue Black.

Returns "---" if no valid measurement is currently available.

Examples VARIable:VALue? "ColorBarsmVCh1"

Query may return:

"ColorBarsmVCh1 699.76 650.52 552.75 501.98 201.89 150.74 52.11
0.49"

ColorBarsmVCh[1..3]Val[1..8]?

Query the value (in mV) resulting from Color Bars measurement for the specified channel and value.

Syntax VARIable:VALue? "ColorBarsmVCh[1..3]Val[1..8]"

Group Results

Arguments None

Related Commands ColorBarsmVCh[1..3]

Returns Returns the specified Color Bars value (in mV).

Values must be in the range: 1..8

Values must designate the following colors:

1-White 2-Yellow 3-Cyan 4-Green 5-Magenta 6-Red 7-Blue 8-Black.

Returns "---" if no valid measurement is currently available

Examples VARIable:VALue? "ColorBarsmVCh2Val6"

Query may return: "ColorBarsmVCh2Val6 -78.89"

ColorBarsSet < setting >

Set or query whether Color Bars is to be measured upon Execute.

Syntax VARIable:VALue "ColorBarsSet", "< setting >"
 VARIable:VALue? "ColorBarsSet"

Group Configuration

Arguments < setting > specifies whether to perform Color Bars measurement upon Execute. Valid values are: OFF, ON, 0, 1

Related Commands Execute
 ReportMeasurements

Returns Query returns 0 or 1 depending on whether ColorBarsSet measurement is selected.

Examples VARIable:VALue "ColorBarsSet", "ON"
 VARIable:VALue? "ColorBarsSet"

Query may return: "ColorBarsSet 1"

ColorSpace < colorspace >

Set or query video color space to use for measurement.

Syntax VARIable:VALue "ColorSpace", "< colorspace >"
 VARIable:VALue? "ColorSpace"

Group Configuration

Arguments < colorspace > specifies color space that is to be set.
 Valid color spaces are: YPbPr, RGB

Returns Query returns the current specified color space

Examples VARIable:VALue "ColorSpace", "YPbPr"
 VARIable:VALue? "ColorSpace"

Query may return: "ColorSpace YPbPr"

DefaultSettings

Command restores default (factory) settings.

Query returns "OK" unless the command is still being processed, in which case it returns "1".

Restores default (factory) settings.

Syntax VARIable:VALue "DefaultSettings", "1"
 VARIable:VALue? "DefaultSettings"

Group Settings

Arguments Valid value is 1.

Returns Query returns "OK" unless the command is still being processed, in which case it returns "1".

Examples VARIable:VALue "DefaultSettings", "1"
 VARIable:VALue? "DefaultSettings"

Query may return: "DefaultSettings OK"

Error < setting >

Command can be used to reset Error to "0".

Query returns the most recent error reported by the application, or "0" if no errors have occurred since Error was last reset.

Initialized to "0" on startup.

Syntax VARIable:VALue "Error" < setting >
 VARIable:VALue? "Error"

Group Miscellaneous

Arguments < setting > resets Error to "0".
 Valid values are: OFF, 0.

Returns Returns the most recent error reported by the application. Returns "0" if no error has occurred since the Error command was last reset. For a listing of all possible errors, refer to Table C-9 on page C-71.

Examples VARIable:VALue "Error", "OFF"
 VARIable:VALue? "Error"

Query may return: "Error No Measurement Selected"

Execute < setting >

Execute/stop the current set measurement(s), or query whether any measurement is currently being executed. If the measurement is already in the mode specified by the setting, the command has no effect. For example, if a measurement is already running and "VARIABLE:VALUE "Execute", "1" is received, the measurement will continue to run.

Syntax VARIABLE:VALUE "Execute", "< setting >"
VARIABLE:VALUE? "Execute"

Group Run

Arguments < setting > Valid settings are: OFF, 0, ON, 1.
OFF is the same as 0, and ON is the same as 1.

Related Commands ChannelDelaySet
ColorBarSet
MultiburstSet
NoiseSet
NonLinearitySet
SyncSet

Returns Query returns 1 if any measurement is currently being executed, otherwise it returns 0.

Examples VARIABLE:VALUE "Execute", "1"
VARIABLE:VALUE? "Execute"

Query may return: "Execute 1"

Format < format >

Set or query video format to use for measurement. No defaults.

If you get the error message, "Invalid Argument", make sure that you specified a valid format.

Syntax	VARIABLE:VALUE "Format", "< format >" VARIABLE:VALUE? "Format"
Group	Configuration
Arguments	< format > specifies format that is to be set. Valid formats are: HD480P60, HD576P50, HD720P60, HD1080I50, HD1080I60, SXGAP60
Returns	Query returns the current specified format.
Examples	VARIABLE:VALUE "Format", "HD480P60" VARIABLE:VALUE? "Format" Query may return: "Format HD1080I60"

ID?

Query the ID/Version of the application.

Syntax VARIable:VALue? "ID"

Group Miscellaneous

Arguments None

Returns Returns the application's ID

Examples VARIable:VALue? "ID"

Query may return: "ID Tek/VM5000HD FV:1.0"

MultiburstAmpdBCh[1..3]?

Query all six amplitude values (in dB) resulting from Multiburst measurement for the specified channel.

Syntax VARIable:VALue? "MultiburstAmpdBCh[1..3]"

Group Results

Arguments None

Related Commands MultiburstAmpdBCh[1..3]Val[1..6]

Returns Returns all six amplitude values (in dB) in burst order.

Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "MultiburstAmpdBCh2"

Query may return:

"MultiburstAmpdBCh2 -0.09 -0.18 -0.14 -0.13 -0.08 -0.02"

MultiburstAmpdBCh[1..3]Val[1..6]?

Query the amplitude (in dB) resulting from Multiburst measurement for the specified channel and value.

Syntax VARIable:VALue? "MultiburstAmpdBCh[1..3]Val[1..6]"

Group Results

Arguments None

Related Commands MultiburstAmpdBCh[1..3]

Returns Returns the specified Multiburst value (in dB).

Returns "---" if no valid measurement is currently available.

Examples VARIable:VALue? "MultiburstAmpdBCh1Val2"

Query may return: "MultiburstAmpdBCh1Val2 -0.26"

MultiburstAverage < samples >

Set or query the number of samples over which to average the Multiburst measurement.

Syntax VARIable:VALue "MultiburstAverage", "< samples >"
 VARIable:VALue? "MultiburstAverage"

Group Setup

Arguments < samples > can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current number of samples for Multiburst measurement.

Examples VARIable:VALue "MultiburstAverage", "1"
 VARIable:VALue? "MultiburstAverage"

Query may return: "MultiburstAverage 8"

MultiburstFlagmVCh[1..3]?

Query the Flag value (in mV) resulting from Multiburst measurement for the specified channel.

Syntax VARIable:VALue? "MultiburstFlagmVCh[1..3]"

Group Results

Arguments None

Returns Returns the Flag value (in mV).

Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "MultiburstFlagmVCh3"

Query may return: "MultiburstFlagmVCh3 428.01"

MultiburstFreqCh[1..3]?

Query all six frequency values (in MHz) resulting from Multiburst measurement for the specified channel.

Syntax VARIable:VALue? "MultiburstFreqCh[1..3]"

Group Results

Arguments None

Related Commands MultiburstFreqCh[1..3]Val[1..6]

Returns Returns all six frequency values (in MHz) in burst order.
Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "MultiburstFreqCh1"

Query may return:
"MultiburstFreqCh1 10.00 12.00 14.00 16.00 18.01 20.00"

MultiburstFreqCh[1..3]Val[1..6]?

Query the frequency (in MHz) resulting from Multiburst measurement for the specified channel and value.

Syntax VARIable:VALue? "MultiburstFreqCh[1..3]Val [1..6]"

Group Results

Arguments None

Related Commands MultiburstFreqCh[1..3]

Returns Returns the specified Multiburst frequency (in MHz).
Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "MultiburstFreqCh1Val2"
Query may return: "MultiburstFreqCh1Val2 12.00"

MultiburstLine < linenumber >

Set or query line number that is to be used for Multiburst measurement.

Syntax VARIable:VALue "MultiburstLine", "< linenumber >"
 VARIable:VALue? "MultiburstLine"

Group Setup

Arguments < linenumber > can be an integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current line number for Multiburst measurement.

Examples VARIable:VALue "MultiburstLine", "200"
 VARIable:VALue? "MultiburstLine"

Query may return: "MultiburstLine 325"

MultiburstSet < setting >

Set or query whether Multiburst is to be measured upon Execute.

Syntax VARIable:VALue "MultiburstSet", "< setting >"
 VARIable:VALue? "MultiburstSet"

Group Configuration

Arguments < setting > specifies whether to perform Multiburst measurement upon Execute. Valid values are: OFF, ON, 0, 1

Related Commands Execute
 ReportMeasurements

Returns Query returns 0 or 1 depending on whether MultiburstSet measurement is selected.

Examples VARIable:VALue "MultiburstSet", "ON"
 VARIable:VALue? "MultiburstSet"

Query may return: "MultiburstSet 1"

NoiseAmpdBCh[1..3]?

Query amplitude value (in dB) resulting from Noise measurement for the specified channel.

Syntax VARIable:VALue? "NoiseAmpdBCh[1..3]"

Group Results

Arguments None

Returns Returns amplitude value (in dB).

Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "NoiseAmpdBCh2"

Query may return: "NoiseAmpdBCh2 66.43"

NoiseAmpmVCh[1..3]?

Query amplitude value (in mV) resulting from a Noise measurement for the specified channel.

Syntax VARIable:VALue? "NoiseAmpmVCh[1..3]"

Group Results

Arguments None

Returns Returns amplitude value (in mV).

Returns "---" if no valid measurement is currently available.

Examples VARIable:VALue? "NoiseAmpmVCh2"

Query may return: "NoiseAmpmVCh2 0.33"

NoiseAverage < samples >

Set or query the number of samples over which to average the Noise measurement.

Syntax VARIable:VALue "NoiseAverage", "< samples >"
 VARIable:VALue? "NoiseAverage"

Group Setup

Arguments < samples > Can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current number of samples for Noise measurement.

Examples VARIable:VALue "NoiseAverage", "1"
 VARIable:VALue? "NoiseAverage"

Query may return: "NoiseAverage 8"

NoiseBW < bandwidth >

Set or query bandwidth of noise filter that is to be used for noise measurement, if the unweighted noise filter is selected.

Syntax VARIABLE:VALUE "NoiseBW", "< bandwidth >"
 VARIABLE:VALUE? "NoiseBW"

Group Setup

Arguments < bandwidth > specifies bandwidth of unweighted noise filter, in Hz. Can be integer or floating point. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Related Commands NoiseFilter

Returns Query returns the current unweighted noise filter bandwidth, in Hz.

Examples VARIABLE:VALUE "NoiseBW", "30000000"
 VARIABLE:VALUE "NoiseBW", "3.2E7"
 VARIABLE:VALUE? "NoiseBW"

Query may return: "NoiseBW 50000000"

NoiseFilter < noisefilter >

Set or query type of noise filter that is to be used for noise measurement.

Syntax VARIable:VALue "NoiseFilter", "< noisefilter >"
 VARIable:VALue? "NoiseFilter"

Group Setup

Arguments < noisefilter > specifies type of noise filter that is to be used for noise measurement. Valid noise filters are: Off, Unified, Unweighted.

Related Commands NoiseBW

Returns Query returns the current specified noise filter.

Examples VARIable:VALue "NoiseFilter", "Unified"
 VARIable:VALue? "NoiseFilter"

Query may return: "NoiseFilter Off"

NoiseLine < linenumber >

Set or query line number that is to be used for Noise measurement.

Syntax VARIable:VALue "NoiseLine", "< linenumber >"
 VARIable:VALue? "NoiseLine"

Group Setup

Arguments < linenumber > Can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current line number for Noise measurement.

Examples VARIable:VALue "NoiseLine", "200"
 VARIable:VALue? "NoiseLine"

Query may return: "NoiseLine 325"

NoiseSet < setting >

Set or query whether Noise is to be measured upon Execute.

Syntax VARIable:VALue "NoiseSet", "< setting >"
 VARIable:VALue? "NoiseSet"

Group Configuration

Arguments < setting > specifies whether to perform Noise measurement upon Execute.
 Valid values are: OFF, ON, 0, 1.

Related Commands Execute
 NoiseMeasurements

Returns Query returns 0 or 1 depending on whether NoiseSet measurement is selected

Examples VARIable:VALue "NoiseSet", "ON"
 VARIable:VALue? "NoiseSet"

Query may return: "NoiseSet 1"

NonLinearityAverage < samples >

Set or query the number of samples over which to average the Non-Linearity measurement.

Syntax VARIable:VALue "NonLinearityAverage", "< samples >"
 VARIable:VALue? "NonLinearityAverage"

Group Setup

Arguments < samples > Can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current number of samples for Non-Linearity measurement.

Examples VARIable:VALue "NonLinearityAverage", "1"
 VARIable:VALue? "NonLinearityAverage"

Query may return: "NonLinearityAverage 8"

NonLinearityLine < linewidth >

Set or query line number that is to be used for Non-Linearity measurement.

Syntax VARIable:VALue "NonLinearityLine", "< linewidth >"
 VARIable:VALue? "NonLinearityLine"

Group Setup

Arguments < linewidth > Can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current line number for Non-Linearity measurement.

Examples VARIable:VALue "NonLinearityLine", "200"
 VARIable:VALue? "NonLinearityLine"

Query may return: "NonLinearityLine 325"

NonLinearityPctCh[1..3]?

Query all six non-linearity values (as a percentage) resulting from Non-Linearity measurement for the specified channel.

Syntax VARIable:VALue? "NonLinearityPctCh[1..3]"

Group Results

Arguments None

Related Commands NonLinearityPctCh[1..3]Max
NonLinearityPctCh[1..3]Val[1..5]

Returns Returns all six non-linearity values (as a percentage) in this order: Maximum
Step1 Step2 Step3 Step4 Step5.

Returns "---" if no valid measurement is currently available

Examples VARIable:VALue? "NonLinearityPctCh3"

Query may return:

"NonLinearityPctCh3 0.82 0.00 0.82 0.69 0.21 0.28"

NonLinearityPctCh[1..3]Max?

Query the maximum non-linearity value (as a percentage) resulting from a Non-Linearity measurement for the specified channel.

Syntax VARIable:VALue? "NonLinearityPctCh[1..3]Max"

Group Results

Arguments None

Related Commands NonLinearityPctCh[1..3]
NonLinearityPctCh[1..3]Val[1..5]

Returns Returns maximum non-linearity value (as a percentage) for specified channel.

Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "NonLinearityPctCh3Max"

Query may return: "NonLinearityPctCh3Max 0.82"

NonLinearityPctCh[1..3]Val[1..5]?

Query the non-linearity value (as a percentage) resulting from a Non-Linearity measurement for the specified channel and step.

Syntax VARIable:VALue? "NonLinearityPctCh[1..3]Val[1..5]"

Group Results

Arguments None

Related Commands NonLinearityPctCh[1..3]
NonLinearityPctCh[1..3]Max

Returns Returns non-linearity value (as a percentage) for specified channel and step.

Returns "---" if no valid measurement is currently available.

Examples VARIable:VALue? "NonLinearityPctCh3Val4"

Query may return: "NonLinearityPctCh3Val4 0.21"

NonLinearitySet < setting >

Set or query whether Non-Linearity is to be measured upon Execute.

Syntax VARIable:VALue "NonLinearitySet", "< setting >"
 VARIable:VALue? "NonLinearitySet"

Group Configuration

Arguments < setting > specifies whether to perform Non-Linearity measurement upon Execute.

Valid values are: OFF, ON, 0, 1.

Returns Query returns 0 or 1 depending on whether NonLinearitySet measurement is selected.

Examples VARIable:VALue "NonLinearitySet", "ON"
 VARIable:VALue? "NonLinearitySet"

Query may return: "NonLinearitySet 1"

OPComplete < setting >

OPComplete is set to “1” whenever a VM5000 Option HD GPIB command has been received and processed and a new command is ready to be processed (except for the resetting of OPComplete itself, which sets OPComplete to “0”).

OPComplete can only be reset to “0” by the user, and it can only be set to “1” when a command has been sent and the next command is ready to be input.

OPComplete is designed to control VM5000 Option HD GPIB scripts by ensuring that the previous command is ready before either (1) querying its value or (2) calling the next command. It should therefore be checked and reset in between each command, and before querying the new setting.

If a command sets its value to the same value that it is currently set to, OPComplete will not be set to “1”. To avoid this, either set Header to “ON”, or use all lowercase arguments for text (such as “hd480p60” and “on”), and floating-point input for numeric values (such as 21.0 instead of 21). This will always cause OPComplete to be set.

Initialized to “0” on startup.

Syntax VARIable:VALue "OPComplete", "< setting >"
 VARIable:VALue? "OPComplete"

Group Miscellaneous

Arguments < setting > - resets OPComplete so it is ready for the next command.
Valid values are: OFF, 0.

Returns Query returns “1” if a command has been completed since OPComplete was last reset, otherwise it returns “0”

Examples VARIable:VALue "OPComplete", "OFF"
 VARIable:VALue? "OPComplete"

Query may return: "OPComplete 1"

A typical general-case usage of OPComplete might be:

```
VARIable:VALue "OPComplete", "OFF"
// reset first so we know it is set to "0"

VARIable:VALue "Command1", "Argument1"
// call first command

While ((VARIable:VALue? "OPComplete") == "0") (
    Wait;
)
// wait till first command is ready before calling next command

// Now repeat the same process for the next command:
VARIable:VALue "OPComplete", "OFF"

// reset first so we know it is set to "0"
VARIable:VALue "Command2", "Argument2"
// call next command

While ((VARIable:VALue? "OPComplete") == "0") (
    Wait;
)
// wait till this command is ready before calling next command
// and so on for subsequent commands
```

RecallSettings < pathstring >

Command recalls settings stored in the specified path/filename.

Query returns “OK” unless the command is still being processed, in which case it returns the current pathstring argument.

If you only specify the filename, the default path “c:\VM5000HD” is used. The file specified in pathstring must have the default extension “.vmset”, or else it will be appended.

If you get the error message, “Invalid Filename”, confirm that you typed the correct path and that your path is no more than 60 characters.

Syntax VARIable:VALue "RecallSettings", "< pathstring >"
 VARIable:VALue? "RecallSettings"

Group Settings

Arguments <pathstring> specifies the path/filename where the setup file is stored. Can either be (1) the full path and filename, or (2) just the filename, and the default path “c:\VM5000HD” will be used. The default extension “.vmset” will be appended if it is not specified. The pathstring must be less than 60 characters in length, otherwise the command may not be completed successfully.

Related Commands SaveSettings

Returns Query returns “OK” unless the command is still being processed, in which case it returns the current pathstring argument.

Examples VARIable:VALue "RecallSettings", "c:\VM5000HD\Tek1.vmset"
 VARIable:VALue "RecallSettings", "Tek2.vmset"
 VARIable:VALue? "RecallSettings"

Query may return: "RecallSettings OK"

ReportGenerate < pathstring >

Command generates a measurement report of the specified type (if a measure has been run and results are available), and saves it in the file specified by pathstring. The type of file (.rtf, .csv or .pdf) is determined by the file extension in the pathstring. If the extension does not match one of these endings, a .pdf file is created by default and “.pdf” is appended to the end of the pathstring.

Query returns “OK” unless the command is still being processed, in which case it returns the current pathstring argument.

If you get the error message “Invalid Filename,” confirm that you typed the correct path and that your path is no more than 60 characters.

Syntax VARIable:VALue "ReportGenerate", "< pathstring >"
 VARIable:VALue? "ReportGenerate"

Group Reports

Arguments <pathstring> path/filename where file is to be stored. Can either be (1) the full path and filename, or (2) just the filename, and the default path “c:\VM5000HD” will be used. The default extension “.pdf” will be appended if it is not specified. The specified directory will be created if it doesn’t currently exist. The pathstring must be less than 60 characters in length, otherwise the command may not be completed successfully.

Related Commands ReportString
 ReportMeasurements

Returns Query returns “OK” unless the command is still being processed, in which case it returns the current pathstring argument.

Examples VARIable:VALue "ReportGenerate", "J:\netpath\colorbars.csv"
 VARIable:VALue "ReportGenerate", "noise02"
 VARIable:VALue? "ReportGenerate"

Query may return: "ReportGenerate OK"

ReportMeasurements < setting >

Set or query the measurements to write to the report when ReportGenerate is called.

Set to "All" when application starts.

Syntax VARIable:VALue "ReportMeasurements", "< measurementmode>"
VARIable:VALue? "ReportMeasurements"

Group Reports

Arguments < measurementmode > specifies the measurements that are to be written to the report when ReportGenerate is called. Valid measurementmode values are All and Selected. All reports all current valid measurements results, while Selected reports only those measurements that are currently set.

Related Commands ChannelDelaySet
ColorBarsSet
MultiburstSet
NoiseSet
NonLinearitySet
ReportGenerate
SyncSet

Returns Query returns the current specified report measurement mode.

Examples VARIable:VALue "ReportMeasurements", "All"
VARIable:VALue? "ReportMeasurements"

Query may return: "ReportMeasurements Selected"

ReportString < string >

Set or query user-specified information to write to the report when ReportGenerate is called.

Initialized to empty string "" on startup.

Syntax VARIable:VALue "ReportString", "< string >"
 VARIable:VALue? "ReportString"

Group Reports

Arguments < string > can be up to 46 characters in length. The comma and double quote characters are not permitted and their usage may result in unexpected program behavior. All other printable characters are permitted.

Related Commands ReportGenerate

Returns Query returns the currently specified report string.

Examples VARIable:VALue "ReportString", "Tested by Joe B - DUT A1"
 VARIable:VALue? "ReportString"

Query may return: "ReportString Tested by Joe B - DUT A1"

If assigning consecutive long strings to ReportString, truncation of the second string may occur if the length of the consecutive strings exceeds a limit (67 characters if Header is ON). For example:

```
VARIable:VALue "ReportString", "This is a long string which has
45 characters"
```

```
VARIable:VALue? "ReportString"
"ReportString This is a long string which has 45 characters"
```

```
VARIable:VALue "ReportString", "This string will be truncated, it
is 45 chars"
```

```
VARIable:VALue? "ReportString"
"ReportString This string will be tr"
```

To avoid this truncation, send a short string to ReportString prior to sending the second string.

```
VARiable:VALue "ReportString", "This is a long string which has  
45 characters"
```

```
VARiable:VALue? "ReportString"  
"ReportString This is a long string which has 45 characters"
```

```
VARiable:VALue "ReportString", "short"
```

```
VARiable:VALue? "ReportString"  
"ReportString short"
```

```
VARiable:VALue "ReportString", "This string won't be truncated,  
it is 46 chars"
```

```
VARiable:VALue? "ReportString"  
"ReportString This string won't be truncated, it is 46 chars"
```


RunMode < runmode >

Set or query the run mode to use for measurement.

Syntax VARIable:VALue "RunMode", "< runmode >"
 VARIable:VALue? "RunMode"

Group Configuration

Arguments < runmode > specifies the run mode that is to be used.
 Valid run modes are: Once, Continuously.

Returns Query returns the currently specified run mode.

Examples VARIable:VALue "RunMode", "Once"
 VARIable:VALue? "RunMode"

Query may return: "RunMode Continuously"

SaveSettings < pathstring >

Command saves current settings in the specified path/filename.

Query returns "OK" unless the command is still being processed, in which case it returns the current pathstring argument.

If you only specify the filename, the default path "c:\VM5000HD" is used. The file will be saved using the default extension ".vmset".

If you get the error message "Invalid Filename," confirm that you typed the correct path and that your path is no more than 60 characters.

Syntax VARIable:VALue "SaveSettings", "< pathstring >"
 VARIable:VALue? "SaveSettings"

Group Settings

Arguments <pathstring> specifies the path/filename where the file is to be stored. Can either be (1) the full path and filename, or (2) just the filename, and the default path "c:\VM5000HD" will be used. The default extension ".vmset" will be appended if it is not specified. The specified directory will be created if it doesn't currently exist. The pathstring must be less than 60 characters in length, otherwise the command may not be completed successfully.

Related Commands RecallSettings

Returns Query returns "OK" unless the command is still being processed, in which case it returns the current pathstring argument.

Examples VARIable:VALue "SaveSettings", "c:\VM5000HD\Tek1.vmset"
 VARIable:VALue "SaveSettings", "Tek2.vmset"
 VARIable:VALue? "SaveSettings"

Query may return: "SaveSettings OK"

SetupAndOrRun < setuprunmode >

Set or query the setup run mode to use for measurement.

Syntax VARIable:VALue "SetupAndOrRun", "< setuprunmode >"
 VARIable:VALue? "SetupAndOrRun"

Group Configuration

Arguments < setuprunmode > specifies how to perform setup when performing a measurement. Valid modes are: SetupAndRun, SetupOnly, RunOnly.

Returns Query returns the current specified setuprunmode.

Examples VARIable:VALue "SetupAndOrRun", "SetupAndRun"
 VARIable:VALue? "SetupAndOrRun"

Query may return: "SetupAndOrRun SetupAndRun"

SyncAverage < samples >

Set or query the number of samples over which to average the Sync measurement.

Syntax VARIable:VALue "SyncAverage", "< samples >"
 VARIable:VALue? "SyncAverage"

Group Setup

Arguments <samples > can be integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current number of samples for Sync measurement.

Examples VARIable:VALue "SyncAverage", "1"
 VARIable:VALue? "SyncAverage"

Query may return: "SyncAverage 8"

SyncLevelsmV?

Query all synchronization levels (in mV) resulting from a Sync measurement.
For Tri-Level Sync, this returns three levels.
For Bi-Level Sync, this returns two levels.

Syntax VARIable:VALue? "SyncLevelsmV"

Group Results

Arguments None

Related Commands SyncLevelsmVVal[1..3]

Returns Returns all synchronization levels (in mV) in this order:
For Tri-Level: FrontPorchLevel NegativeSyncLevel PositiveSyncLevel.
For Bi-Level: FrontPorchLevel SyncLevel.

Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "SyncLevelsmV"

Query may return: "SyncLevelsmV 0.89 -298.31 299.11"

SyncLevelsmVVal[1..3]?

Query the specified synchronization level (in mV) resulting from a Sync measurement.

Syntax VARIable:VALue? "SyncLevelsmVVal[1..3]"

Group Results

Arguments None

Related Commands SyncLevelsmV

Returns Returns specified synchronization level (in mV).

Values must be in the following ranges:

For Tri-Level, 1..3

For Bi-Level, 1..2

Values must designate the following levels:

For Tri-Level: 1-FrontPorchLevel, 2-NegativeSyncLevel, 3-PositiveSyncLevel.

For Bi-Level: 1-FrontPorchLevel, 2-SyncLevel.

Returns "---" if no valid measurement currently available

Examples VARIable:VALue? "SyncLevelsmVVal3"

Query may return: "SyncLevelsmVVal3 299.11"

SyncLine < linenumber >

Set or query line number that is to be used for Sync measurement.

Syntax VARIable:VALue "SyncLine", "< linenumber >"
 VARIable:VALue? "SyncLine"

Group Setup

Arguments < linenumber > can be an integer or floating point, but will be rounded to the next lowest integer. Values outside the range will be adjusted to be within range. Floating point notation is allowed.

Returns Query returns the current line number for Sync measurement.

Examples VARIable:VALue "SyncLine", "200"
 VARIable:VALue? "SyncLine"

Query may return: "SyncLine 325"

SyncSet < setting >

Set or query whether Sync is to be measured upon Execute.

Syntax VARIable:VALue "SyncSet", "< setting >"
 VARIable:VALue? "SyncSet"

Group Configuration

Arguments < setting > specifies whether to perform Sync measurement upon Execute.
Valid values are: OFF, ON, 0, 1.

Related Commands Execute
 ReportMeasurements

Returns Query returns 0 or 1 depending on whether SyncSet measurement is selected.

Examples VARIable:VALue "SyncSet", "ON"
 VARIable:VALue? "SyncSet"

Query may return: "SyncSet 1"

SyncTimes?

Query all synchronization times (in nanoseconds) resulting from a Sync measurement.

For Tri-Level Sync, this returns seven times.
For Bi-Level Sync, this returns five times.

Syntax VARIable:VALue? "SyncTimes"

Group Results

Arguments None

Related Commands SyncTimesVal[1..7]

Returns Returns all synchronization times (in nanoseconds) in the order:
For Tri-Level: FrontPorch NegativeSyncFall NegativeSyncWidth SyncRise
PositiveSyncWidth PositiveSyncFall BackPorch.
For Bi-Level: FrontPorch NegativeSyncFall NegativeSyncWidth SyncRise
BackPorch.

Returns "---" if no valid measurement currently available

Examples VARIable:VALue? "SyncTimes"

Query may return:
"SyncTimes 3822.39 59.03 592.01 52.61 590.40 55.24 1995.19"

SyncTimesVal[1..7]?

Query the specified synchronization time (in nanoseconds) resulting from Sync measurement.

Syntax VARIable:VALue? "SyncTimesVal [1..7]"

Group Results

Arguments None

Related Commands SyncTimes

Returns Returns specified synchronization time (in nanoseconds).

Values must be in these ranges:

For Tri-Level 1..7

For Bi-Level 1..5

Values must designate the following times:

For Tri-Level: 1-FrontPorch, 2-NegativeSyncFall, 3-NegativeSyncWidth, 4-SyncRise, 5-PositiveSyncWidth, 6-PositiveSyncFall, 7-BackPorch.

For Bi-Level: 1-FrontPorch, 2-NegativeSyncFall, 3-NegativeSyncWidth, 4-SyncRise, 5-BackPorch.

Returns "---" if no valid measurement currently available.

Examples VARIable:VALue? "SyncTimesVal2"

Query may return: "SyncTimesVal2 59.03"

Trigger < trigger >

Set or query video trigger to use for measurement.

Syntax VARIable:VALue "Trigger", "< trigger >"
 VARIable:VALue? "Trigger"

Group Configuration

Arguments < trigger > specifies trigger that is to be used.
 Valid triggers are: Ch1, Ch4.

Returns Query returns the current specified trigger.

Examples VARIable:VALue "Trigger", "Ch4"
 VARIable:VALue? "Trigger"

Query may return: "Trigger Ch4"

WarningReportingMeasure < setting >

Set or query whether the instrument displays a measurement setup problem warning dialog on the instrument screen.

Syntax VARIable:VALue "WarningReportingMeasure", "< setting >"
 VARIable:VALue? "WarningReportingMeasure"

Group Configuration

Arguments < setting > Valid settings are: OFF, ON, 0, 1.
 OFF is the same as 0, and ON is the same as 1.

Related Commands WarningReportResults
 WarningReportSignal

Returns Query returns the current specified setting.

Examples VARIable:VALue "WarningReportingMeasure", "ON"
 VARIable:VALue? "WarningReportingMeasure"

 Query may return: "WarningReportingMeasure 0"

WarningReportingResults < setting >

Set or query whether the instrument displays a measurement results warning dialog on the instrument screen.

Syntax VARIable:VALue "WarningReportingResults", "< setting >"
 VARIable:VALue? "WarningReportingResults"

Group Configuration

Arguments < setting > valid settings are: OFF, 0, ON, 1.
 OFF is the same as 0, and ON is the same as 1.

Related Commands WarningReportingMeasure
 WarningReportingSignal

Returns Query returns the current specified setting.

Examples VARIable:VALue "WarningReportingResults", "ON"
 VARIable:VALue? "WarningReportingResults"

Query may return: "WarningReportingResults 0"

WarningReportingSignal < setting >

Set or query whether the instrument displays an input signal problem warning dialog on the instrument screen.

Syntax VARIable:VALue "WarningReportingSignal", "< setting >"
 VARIable:VALue? "WarningReportingSignal"

Group Configuration

Arguments < setting > valid settings are: OFF, 0, ON, 1.
 OFF is the same as 0, and ON is the same as 1.

Related Commands WarningReportingMeasure
 WarningReportingResults

Returns Query returns the current specified setting.

Examples VARIable:VALue "WarningReportingSignal", "ON"
 VARIable:VALue? "WarningReportingSignal"

 Query may return: "WarningReportingSignal 0"

Warning < setting >

Command can be used to reset Warning to "0". Query returns the most recent warning reported by the application, or "0" if no warning have occurred since Warning was last reset. All warnings (Measurement, Signal, and Results) will be reported.

Initialized to "0" on startup.

Syntax VARIable:VALue "Warning" < setting >
 VARIable:VALue? "Warning"

Group Miscellaneous

Arguments < setting > resets Warning to 0.
 Valid values are: OFF, 0.

Returns Returns the most recent warning reported by the application. Returns "0" if no warning has occurred since the Warning command was last reset. For a listing of all possible warnings, refer to Table C-8 on page C-70.

Examples VARIable:VALue "Warning", "OFF"
 VARIable:VALue? "Warning"

Query may return:
"Warning Color Bars: Back Porch Reference Questionable"

Warning and Error Messages

Tables C-8 and C-9 list the warning and error messages you could see.

Table C-8: Warning messages

Number	Text	Possible causes	Operation where it may occur
1	Acquisition Problem	The instrument cannot trigger or the signal levels are out of range.	All measurements
2	Channel Delay: Channel <x> & <y>, Correlation Too Low	You may have the wrong line in the matrix signal, a distorted signal, or an inappropriate input signal with too few transitions.	Measuring Channel Delay
3	Channel Delay: Disjoint Correlations Among Channels...	There is a possible group delay mismatch among channels, or there is an inappropriate signal source.	Measuring Channel Delay
4	Color Bars: <Color> Bar Not Found	You may have the wrong line in the matrix signal, a distorted signal, an incorrect format selected, channels connected in the wrong order, the wrong colorimetry, or excessive cropping of the signal.	Measuring Color Bars
5	Color Bars: Back Porch Reference Questionable	The signal is distorted.	Measuring Color Bars
6	Multiburst: Signal Change: <freq1> -> <freq2> MHz	You may have low signal levels, an incorrect signal, or a change in the signal.	Measuring Multiburst
7	Multiburst: Individual Channel Errors: Channel <x>: Flag <= 0 mV	The signal is distorted or a flag is missing in the signal.	Measuring Multiburst
8	Multiburst: Individual Channel Errors: Channel <x>: burst <n>: not detected	You may have low signal levels, distorted signals, an input signal with less than six frequency packets, or excessive cropping of the signal.	Measuring Multiburst
9	Multiburst: Invalid results for all channels	You may have the wrong line in the matrix signal, an inappropriate input signal, or an incorrect configuration.	Measuring Multiburst
10	Noise: Signal Change: Chan <x>	The signal changed during measurement.	Measuring Noise
11	Noise: Invalid results for all channels.	You may have the wrong line in the matrix signal, an inappropriate input signal, or an incorrect configuration.	Measuring Noise
12	Nonlinearity: Invalid Results: Channel <x>: No ramp or step signal found	You may have the wrong line in the matrix signal or an inappropriate input signal.	Measuring NonLinearity
13	Nonlinearity: Signal Change: Channel <x>: ...	The signal changed during measurement.	Measuring NonLinearity
14	Sync Measurements Inconclusive	The instrument could not find a proper sync, the wrong format was selected, or the signal is distorted.	Measuring Sync

Table C-8: Warning messages (Cont.)

Number	Text	Possible causes	Operation where it may occur
15	Sync Measurement: <n> Not Found	The instrument could not find a proper sync.	Measuring Sync
16	Writing over file <filename>	The instrument is writing over a file that previously existed.	Recalling settings; Generating a report

Table C-9: Error messages

Number	Text	Possible causes	Operation where it may occur
1	File Name Error: File doesn't exist: <filename>	The selected .vmset file doesn't exist. (You need to use the full path if the file is not in the directory C:\VM5000HD.)	Recalling settings
2	Cannot write directory: file already exists: <filename>	You need to rename <filename> so that the directory can be written.	Saving settings; Generating a report
3	File Name Error. Invalid character(s) in file name	There are invalid characters in the filename. (Refer to the command structure description on page C-1.)	Saving settings; Generating a report
4	No Measurement Selected	No measurements are selected in the Configuration > Measurements menu.	Executing a measure; Generating a report
5	Cannot create Report. Not all selected measures have been Run	Need to run a measurement and wait until it completes before generating a report.	Generating a report
6	Invalid Filename	An invalid or non-existing file was used when performing the operation. Refer to the command structure description on page C-1. Also, you need to use the full path if the file is not in the directory C:\VM5000HD.	RecallSettings; SaveSettings; ReportGenerate (only when called via GPIB)
7	Invalid Argument	An inappropriate argument was used for the particular GPIB command.	All GPIB commands
8	Command Overflow	The GPIB commands were sent in too rapidly to the instrument. Increase the delay time between commands to prevent this problem (recommended 100 milliseconds), or use handshaking with OPCComplete.	Any time GPIB commands are sent in too rapidly
9	Command Missed	Under certain configurations, a command can occasionally fail to be processed by the instrument. This error suggests that a command sent in the last second may not have been processed, so you should return to a recent (known) configuration and re-send the most recent commands.	Sending a GPIB command

Appendix D: Cleaning

Use these procedures to clean your instrument. If additional cleaning is required, have your instrument serviced by qualified service personnel.

Exterior Cleaning

Clean the exterior surfaces of the chassis with a dry lint-free cloth or a soft-bristle brush. If any dirt remains, use a cloth or swab dipped in a 75% isopropyl alcohol solution. Use a swab to clean narrow spaces around controls and connectors. Do not use abrasive compounds on any part of the chassis.

Clean the On/Standby switch using a dampened cleaning towel. Do not spray or wet the switch directly.



CAUTION. Do not use chemical cleaning agents that might damage the plastics used in this instrument. Use only deionized water when cleaning the front-panel buttons. Use a 75% isopropyl alcohol solution as a cleaner and rinse with deionized water. Before using any other type of cleaner, consult your Tektronix Service Center or representative.

To prevent getting moisture inside the instrument during external cleaning, use only enough liquid to dampen the cloth or applicator.

Flat Panel Display Cleaning

The display is soft plastic and must be treated with care during cleaning.



CAUTION. Improper cleaning agents or methods can damage the flat panel display.

Do not use abrasive cleaners or commercial glass cleaners to clean the display surface.

Do not spray liquids directly on the display surface.

Do not scrub the display with excessive force.

Clean the flat panel display surface by gently rubbing the display with a clean-room wipe (such as Wypall Medium Duty Wipes, #05701, available from Kimberly-Clark Corporation).



CAUTION. *To prevent getting moisture inside the instrument during external cleaning, use only enough liquid to dampen the cloth or applicator.*

If the display is very dirty, moisten the wipe with distilled water or a 75% isopropyl alcohol solution and gently rub the display surface. Avoid using excess force or you may damage the plastic display surface.

Appendix E: Rebuilding the Hard Drive

If you need to rebuild the hard drive, you must install software from three CDs in the following order:

1. Follow the directions in the CD jewel-case booklet to install the Operating System Restore CD, 063-3693-XX.
2. Follow the directions in the CD jewel-case booklet to install the TDS5000B Product Software CD, 063-3692-XX.
3. Install the VM5000 Option HD application CD, 063-3768-XX.
4. Follow the online instructions.

When asked, enter your option key information from the sticker on the back of your instrument.

Appendix F: Signal Source Disks

The Signal Source Disks consists of four CDs and two DVDs that ship with the VM5000 Option HD as a standard accessory. These disks contain Matrix test pattern signal source files in a number of video formats. See page 2-6 for information on the Matrix test pattern. Table F-1 lists the signal source disks.

Table F-1: Signal Source Disks

Title	Tektronix part number
Baseband Test Signals	063-3660-XX
ATSC Transport Streams	063-3661-XX
Advanced TV Elementary Streams	063-3662-XX
Standard Definition TV Elementary Streams	063-3663-XX
480 Line DVD	063-3664-XX
576 Line DVD	063-3665-XX

Baseband Test Signals CD

The Baseband Test Signals disk (Tektronix part number 063-3660-XX) contains files for generating baseband test signals. There are two directories:

- The PC directory contains an SXGA sub-directory that contains a 1280 X 1024 bitmap image file, which you can open with MS Paint on a PC and display the Matrix test pattern at 1280 x 1024 resolution at a 60 Hz horizontal refresh rate. See page 1-15 for instructions on how to use the SXGA Matrix bitmap file.
- The TG700 directory contains setup (.dnl) files for generating Matrix test signals using the Tektronix TG700 TV Signal Generator Platform. Table F-2 lists the available image format standard .dnl setup files.

Table F-2: Available TG700 DNL signal format files

Image format	Field rate	TG700 module	Color space	Signal file name
480p (525 total lines)	59.94	AVG7	RGB	525PSGBR.DNL
			YP _b P _r	S525PY.DNL
576p (625 total lines)	50	AVG7	RGB	625PSGBR.DNL
			YP _b P _r	S625PY.DNL

Table F-2: Available TG700 DNL signal format files (Cont.)

Image format	Field rate	TG700 module	Color space	Signal file name
720p	59.94	AWVG7	RGB	72059PG.DNL
			YP _b P _r	72059PY.DNL
1080i	50	AWVG7	RGB	108050IG.DNL
			YP _b P _r	108050IY.DNL
1080i	59.94	AWVG7	RGB	108059TG.DNL
			YP _b P _r	108059IY.DNL

To use the TG700 .dnl setup files, copy the required file or files to a PC. Then use the communication program that came with the TG700 to move the setup files over your network from the PC to the TG700 instrument. Figure F-1 shows a typical test signal setup using the TG700 instrument as the signal source.

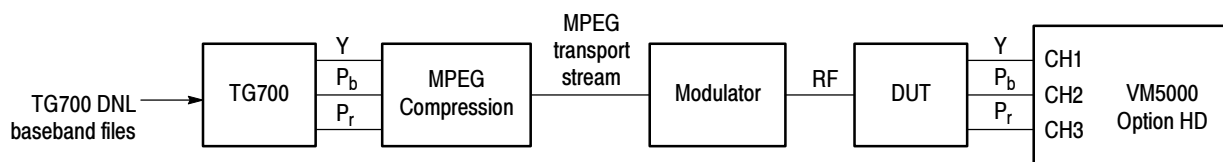


Figure F-1: Using TG700 baseband test signals

ATSC Transport Stream CD

The ATSC Transport Streams disk (Tektronix part number 063-3661-XX) contains files for playout on an MPEG player (such as the Tektronix MTX100 MPEG Recorder and Player) to generate Matrix pattern compressed ATSC transport stream test signals for 480, 720, and 1080 standards. Table F-3 lists the available image format standard .trp setup files.

Table F-3: Available MXT100 .trp signal setup files

Image format	Field rate	MTX100 setup file(s)	Associated VM5000 Option HD setup file
480p	59.94	Tek480pMatrix.trp Tek480p16x9Matrix.trp	Tek480pMatrix.vmset
720p	59.94	Tek720pMatrix.trp	Tek720pMatrix.vmset
1080i	59.94	Tek1080iMatrix.trp	Tek1080iMatrix.vmset

The disk also contains some or all of the following:

- Readme files that contain detailed information on each signal setup file. You should view the readme files before using a signal setup file.
- The .vmset files that you recall into the VM5000 Option HD instrument to configure the correct default line number values for each measurement. See page 2-16 for instructions on how to recall VM5000 Option HD instruments setups.

NOTE. You must use the associated .vmset file to configure the VM5000 Option HD before taking measurements from test signals generated using a .trp setup file.

- WFM700 directories that contain .bmp-format screen captures from the Tektronix WFM700 series Waveform Monitor, showing individual lines and channels of the Matrix test signal 1 minute video loop, for a particular format.

To use the MTX100 .trp setup files, insert the disk into the MTX00. Refer to the *MTX100 MPEG Recorder and Player User* manual for information on loading instrument setup files. Figure F-2 shows a typical test signal setup using the MTX100 instrument as the signal source.

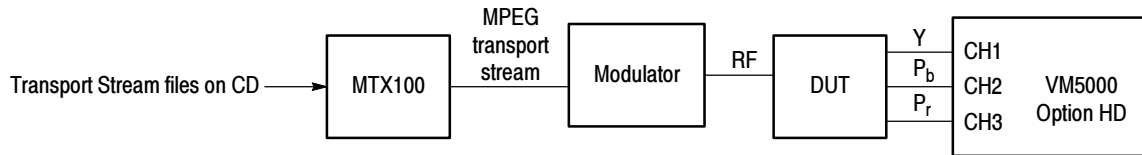


Figure F-2: Using ATSC transport stream signals

Advanced TV Elementary Streams CD

Standard Definition TV Elementary Streams CD

The Advanced TV Elementary Streams disk (Tektronix part number 063-3662-XX) and the The Standard Definition TV Elementary Streams disk (Tektronix part number 063-3663-XX) contain MPEG2-compressed elementary stream files. You use these files with a transport stream multiplexor to build advanced TV or standard definition TV transport streams. Tables F-4 and F-5 list the available elementary stream formats.

Table F-4: Available Advanced TV Elementary Streams

Image format	Field rate	File	Ratio	Associated VM5000 Option HD setup file
480p	59.94	Tek480pMatrix.mpg	4:3	Tek480pMatrix.vmsset
		Tek480p16x9Matrix.mpg	16:9	
720p	59.94	Tek720pMatrix.mpg		Tek720pMatrix.vmsset
1080i	50	Tek1080i50Matrix.mpg		Tek1080iMatrix.vmsset
	59.94	Tek1080iMatrix.mpg		

Table F-5: Available Standard Definition TV Elementary Streams

Image format	Field rate	File	Ratio	Associated VM5000 Option HD setup file
480i	59.94	Tek480iMatrix.mpg	4:3	none
		Tek480i16x9Matrix.mpg	16:9	
576i	59.94	Tek576iMatrix.mpg	4:3	none
		Tek576i16x9Matrix.mpg	16:9	

The disk also contains some or all of the following:

- Readme files that contain detailed information on each signal setup file. You should view the readme files before using a signal setup file.
- The .vmset files that you recall into the VM5000 Option HD instrument to configure the correct default line number values for each measurement. See page 2-16 for instructions on how to recall VM5000 Option HD instruments setups.

NOTE. You must use the associated .vmset file that is on the same disk to configure the VM5000 Option HD before taking measurements that use the elementary stream signals.

To use the elementary stream files, copy the appropriate files into your transport stream multiplexor. Figure F-3 shows a typical elementary stream test setup.

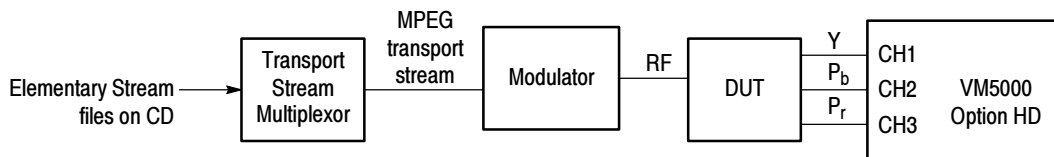


Figure F-3: Using elementary stream signals

480 & 576 Line DVDs

The 480 Line DVD (Tektronix part number 063-3664-XX) and 576 Line DVD (Tektronix part number 063-3665-XX), both generate 60-second Matrix pattern test signals for use with the VM5000 Option HD instrument. The DVD files are available in the formats listed in Table F-6.

Table F-6: Available formats of DVD files

DVD	Image format	Field rate	Program/Track	Ratio
480 Line	480i	59.94	1	16:9
			2	4:3
576 Line	576i	50	1	16:9
			2	4:3

To use the DVD, insert the appropriate DVD into the player, then select the appropriate program/track for the ratio. Figure F-4 shows the typical setup for testing DVD players.

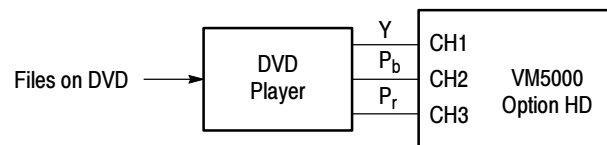


Figure F-4: Using DVD signals

NOTE. The DVD files are in interlace format. The playback device must be set to progressive mode (480p or 576p) before sending signals to the VM5000 Option HD instrument.



Index

Index

Numbers

- 3-wire composite sync setup, 2-2, 2-3
- 4-wire with separate sync setup, 2-4
- 75 Ohm termination, CH4, 2-4

A

- Access the Windows desktop, 2-8
- Accessories, 1-19
 - connecting peripherals, 1-7
 - optional, 1-21
 - probes, 1-3-1-4
 - standard, 1-20
- Address, Tektronix, xi
- Adjusting display contrast, 1-12
- Algorithm descriptions. *See* Measurements, detailed information
- All button, 2-18, 3-11
- Ambient temperature, A-1
- Amplitude change, re-do auto scaling, 3-7
- App button, 2-8
- Application display, default, 2-7
- Application software version number, 3-12
- Application view area, 2-8
- Applications, Microsoft, 1-11
- Auto Scale
 - buttons, 2-12
 - re-do, 3-7
- AutoScale, C-8
- Averages, 3-13
 - interactions with results, 3-8
 - interactions with Run Mode, 3-8

B

- Backing up user files, 1-9
- Baseband files, Matrix test pattern, F-1
- Buttons
 - All, 2-18, 3-11
 - App (restore hidden application), 2-8
 - Auto Scale On/Off, 2-12
 - color space type, 2-9
 - Continuously, 2-12, 3-7
 - CSV, 2-17, 3-11
 - Exit, 2-8
 - Generate Report, 2-18
 - Hide, 2-8
 - input signal format, 2-9

- instrument On/Standby, 2-7
- Once, 2-12, 3-7
- Open (load measurement settings), 2-16
- PDF, 2-17, 3-11
- RTF, 2-17, 3-11
- Run, 2-8
- Run Mode, 2-12, 3-7
- Run Only, 2-11, 3-6
- Save (measurement settings), 2-15
- Selected, 2-18, 3-11
- Setup & Run, 2-11, 3-6
- Setup Only, 2-11, 3-6
- Stop, 2-8
- sync signal trigger channel select, 2-12

C

- CD-ROMs, product software, 1-10
- Certifications and compliances, A-16
- Changing measurement settings, 2-14
- Channel Delay measurement, detailed information, 3-14
- Channel input and vertical specifications, A-2
- ChannelDelayAll?, C-9
- ChannelDelayAverage, C-10
- ChannelDelayCh1Ch2?, C-11
- ChannelDelayCh1Ch3?, C-12
- ChannelDelayCh2Ch3?, C-13
- ChannelDelayLine, C-14
- ChannelDelaySet, C-15
- Cleaning
 - exterior, D-1
 - flat panel display, D-1
- Color Bars measurement, detailed information, 3-16
- ColorBarsAverage, C-16
- ColorBarsLine, C-17
- ColorBarsmVCh[1..3], C-18
- ColorBarsmVCh[1..3]Val[1..8], C-19
- ColorBarsSet, C-20
- ColorSpace, C-21
- Commands, C-8
 - See also* Remote commands
- Compressed elementary stream files, F-5
- Compressed transport stream files, F-3
- Configuration commands, C-4
- Configuration menu, 3-5
- Connecting input signals, 2-2
- Connecting peripherals, 1-7
- Connecting to a network, 1-11

Contacting Tektronix, xi
Creating an emergency startup disk, 1-9
CSV, 2-17, 3-11

D

Data storage specifications, A-13
Default application display, 2-7
DefaultSettings, C-22
Description
 key features, 1-1
 product, 1-1
Desktop, accessing windows, 2-8
Display specifications, A-11
DNL files, Matrix test pattern, F-1
Documentation, related, x
DVD files, Matrix test pattern, F-7
Dynamic range, maximize by autoscaling, 3-7

E

Elementary stream files, Matrix test pattern, F-5
Environment requirements, 1-6
Environmental specifications, A-15
Error, C-23
Error and warning messages, C-70
Execute, C-24
Exit button, 2-8
Exiting the application, 1-11
Exterior cleaning, D-1

F

File menu, 3-3
Files
 .vmset, 3-3
 Matrix test pattern signal source, F-1
 reports, 3-11
Filter settings, 3-8
Firmware, upgrade, 1-3
Flat panel display cleaning, D-1
Format, C-25
Format, input signal, 2-9
Function reference, 3-3

G

Generate Report menu, 3-11
GPIB commands. *See* Remote commands
GPIB operation, avoiding message box interruptions,
 3-7

H

Help, 3-12
Hide button, 2-8
Horizontal and acquisition system specifications, A-7

I

ID?, C-26
Input Matrix test pattern files
 for a DVD player, F-7
 for MTX100, F-3
 for TG700, F-1
 for transport stream multiplexor, F-5
Input signal. *See* Matrix test pattern; Measurements,
 detailed information
Input signal connection requirements, 2-1
Input signal format, 2-9
Input signal format view, 2-9
Input signal setups
 3-wire composite sync, 2-2, 2-3
 4-wire with separate sync, 2-4
 PC video card, 2-5
Input/output port specifications, A-12
Installation, 1-5
 incoming inspection procedure, 1-13
 software installation, 1-10
Installing system software, E-1
Interruptions by message boxes, avoiding, 3-7
Intrepreting results. *See* Measurements, detailed
 information
Introduction, to this manual, ix

K

Key features, 1-1

L

LCD display contrast, 1-12
Line Number, 3-8
Line Number defaults in .vmset file, 3-3
Loading saved measurement setups, 2-16

M

Manuals
 part numbers, 1-20
 related, x
Matrix signal line numbers, 3-13

Matrix test pattern
 formats, F-1
 picture, 2-6
 Matrix test signal, matching setup file, 3-3
 Measurement settings, changing, 2-14
 Measurement setups
 recalling, 2-16
 saving, 2-15
 Measurement steps overview, 2-9
 Measurements
 detailed information, 3-13
 measurements to report, 2-18, 3-11
 overview, 3-8
 report formats, 2-17, 3-11
 reports, 2-17
 saving results (reports) to a file, 2-17
 selecting, 2-10
 setting run-time options, 2-11
 Mechanical specifications, A-14
 Menu bar, 2-8
 Menu descriptions, 3-3
 Message boxes, avoiding interruptions, 3-7
 Messages, C-70
 Minimizing the application and main display, 2-8
 Miscellaneous commands, C-4
 MTX100 files, Matrix test pattern, F-3
 Multiburst measurement, detailed information, 3-17
 MultiburstAmpdBCh[1..3], C-27
 MultiburstAmpdBCh[1..3]Val[1..6], C-28
 MultiburstAverage, C-29
 MultiburstFlagmVCh[1..3], C-30
 MultiburstFreqCh[1..3], C-31
 MultiburstFreqCh[1..3]Val[1..6], C-32
 MultiburstLine, C-33
 MultiburstSet, C-34
 Multiplexor files, Matrix test pattern, F-5

N

Network access, 1-11
 Noise measurement, detailed information, 3-19
 NoiseAmpdBCh[1..3], C-35
 NoiseAmpmVCh[1..3], C-36
 NoiseAverage, C-37
 NoiseBW, C-38
 NoiseFilter, C-39
 NoiseLine, C-40
 NoiseSet, C-41
 Non Linearity measurement, detailed information, 3-20
 NonLinearityAverage, C-42
 NonLinearityLine, C-43
 NonLinearityPctCh[1..3], C-44

NonLinearityPctCh[1..3]Max?, C-45
 NonLinearityPctCh[1..3]Val[1..5]?, C-46
 NonLinearitySet, C-47

O

On/Standby switch, 1-8
 Online help, 3-12
 OPComplete, C-48
 Open (load measurement settings) button, 2-16
 Opening, .vmset files, 3-3
 Operating requirements, 1-6
 Optimizing for production line testing, auto scale Off,
 3-7
 Option SS, F-1
 Optional accessories, 1-21
 Options, 1-19
 Out of range, preventing by autoscaling, 3-7

P

PC video card test setup, 2-5
 PDF, 2-17, 3-11
 Performance verification
 functional tests, 1-14
 self tests, 1-13
 Peripherals, connecting, 1-7
 Phone number, Tektronix, xi
 Power source specifications, A-14
 Powering off, 1-8
 Powering on, 1-8
 Probes, supported, 1-3
 Product
 accessories. *See* Accessories
 description, 1-1
 models, 1-1
 unpacking, 1-5
 Product features, 1-1
 Product support, contact information, xi

Q

Quitting the application, 1-11

R

Re-do auto scaling, 3-7
 Rebuilding the Hard Drive, E-1
 Recalling measurement setups, 2-16, 3-3
 RecallSettings, C-50

- Reinstalling the system software, E-1
- Related documentation, x
- Release notes, 1-10
- Remote commands, C-1
 - command descriptions, C-8
 - startup and exit, C-3
- Report generating, menu descriptions, 3-11
- ReportGenerate, C-51
- Reports, viewing on the MS Windows desktop, 2-8
- Reports commands, C-5
- ReportString, C-52, C-53
- Restore the application when hidden, 2-8
- Results appear as dashes, 3-5
- Results commands, C-5
- Results menu, 3-8
- RTF, 2-17, 3-11
- Run button, 2-8
- Run commands, C-6
- Run Mode, 3-6
 - buttons, 2-12
 - interactions with Average setting, 3-8
- Run Only button, 2-11, 3-6
- RunMode, C-55
- Running the application, 2-7

S

- SaveSettings, C-56
- Saving measurement setups, 2-15
- Selected button, generating reports, 2-18, 3-11
- Selecting measurements, 2-10
- Serial, command descriptions, C-8
- Service support, contact information, xi
- Setting run-time options, 2-11
- Settings commands, C-6
- Setup & Run button, 2-11, 3-6
- Setup commands, C-6
- Setup for functional tests, 2-5
- Setup Only button, 2-11, 3-6
- SetupAndOrRun, C-57
- Show the application when hidden, 2-8
- Shutdown, 1-8
- Signal amplitude change, auto scaling, 3-7
- Signal path compensation, 1-14, A-1
- Signal sources
 - matrix files, F-1
 - non-matrix. *See* Measurements, detailed information
- Site considerations, 1-6
- Software, reinstallation, E-1
- Software installation, 1-10
- Software version number, 3-12
- Space requirements, 1-6

- Specifications, A-1
 - certifications and compliances, A-16
 - channel input and vertical, A-2
 - data storage , A-13
 - display, A-11
 - environmental, A-15
 - horizontal and acquisition system, A-7
 - input/output port , A-12
 - mechanical, A-14
 - power source, A-14
 - trigger, A-8
 - video measurements, A-1
- Standard accessories, 1-20
- Starting the application, 2-7
- Startup disk, creating, 1-9
- Stop button, 2-8
- SXGA/60 bitmapped file, Matrix test pattern, F-1
- Sync measurement, detailed information, 3-21
- Sync signal trigger channel buttons, 2-12
- SyncAverage, C-58
- SyncLevelsmV?, C-59
- SyncLevelsmVVal[1..3]?, C-60
- SyncLine, C-61
- SyncSet, C-62
- SyncTimes?, C-63
- SyncTimesVal[1..7]?, C-64
- Syntax, C-1
- System diagnostics menu, 1-13

T

- Taking a measurement, 2-13
- Taking measurements overview, 2-9
- Technical support, contact information, xi
- Tektronix, contacting, xi
- Termination, 75 Ohm, CH4, 2-4
- Test signal. *See* Matrix test pattern
- TG700 DNL files, Matrix test pattern, F-1
- Transport stream files, Matrix test pattern, F-3
- Trigger, C-65
- Trigger specifications, A-8

U

- Unhiding hidden application, 2-8
- Upgrade, firmware, 1-3
- URL, Tektronix, xi
- USB devices, 1-7
- User files, backing up, 1-9
- User interface description, 2-8

Utilities menu

- Generate Report, 3-11
- Instrument Calibration, 1-14
- Instrument Diagnostics, 1-13

V

- Verification, incoming inspection procedure, 1-13
- Version number, 3-12
- Vertical scale autoscaling, 3-7
- Video specifications, A-1
- Viewing measurement results, 2-13
- Viewing reports on the desktop, 2-8
- VMSET files, recalling, 3-3

W

- Warning, C-69
- Warning and error messages, C-70
- Warning message boxes, turn off or on, 3-7
- Warning message reporting, 2-12
- WarningReportingMeasure, C-66
- WarningReportingResults, C-67
- WarningReportingSignal, C-68
- Web site address, Tektronix, xi
- Windows desktop, accessing, 2-8
- Windows operating system, backup tool, 1-9

