



# **Eight-Channel Low Pass Filter Signal Conditioning Plug-on VT1512A**

---

## **User's Manual**

The VT1512A manual also applies to Agilent/HP E1413Bs as Agilent/HP E1413 Option 22.

Enclosed is the User's Manual for the VT1512A Signal Conditioning Plug-on. Insert this manual in your VT1413C manual behind the "Signal Conditioning Plug-ons" divider.



Copyright © VXI Technology, Inc., 2003



# VT1512A

## Eight-Channel Low Pass Filter Signal Conditioning Plug-on

---

### Introduction

The VT1512A is a Signal Conditioning Plug-on that provides eight fixed low-pass filters with a 3 dB cutoff frequency of 25 Hz. Also provided is input over-voltage protection and open transducer detection on each channel.

### About this Manual

This manual shows you how to control the Signal Conditioning Plug-on (SCP) using SCPI commands as well as Register-Based commands, and explains the capabilities of this SCP. Finally, it covers specifications for this SCP. The contents of this manual are:

- Installation ..... 1
- Identifying the Plug-on ..... 1
- Connecting To The Terminal Module ..... 2
- Programming With SCPI Commands ..... 4
- Programming With Register Commands ..... 6
- Specifications ..... 8

### Installation

Installation for this Plug-on is common to several others and is covered in Chapters 1 and 2 of your VT1413C or Agilent/HP E1313 manuals.

### Identifying the Plug-on

You'll find the VXI Technology part number on the connector side of the SCP to the left of the serial number bar code. For the VT1512A, the part number is: VT1512A.

# Connecting To The Terminal Module

This section shows how to make connections to the Terminal Module.

The SCP connections for the Terminal Modules are shown on the stick-on labels that came with the SCP. Use the appropriate label for the type of Terminal Module you have. The connections and appropriate stickers are as follows:

- For VT1413C and above Terminal Modules, use stickers for VT1512A SCPs. The connections are shown in Figure 1.
- For Agilent/HP E1313 Terminal Modules, use stickers for VT1512A SCPs. The connections are shown in Figures 2 and 3.
- For Agilent/HP E1413B and below Terminal Modules, use stickers for Agilent/HP E1413 Option 12 SCPs. The connections are shown in Figure 4.



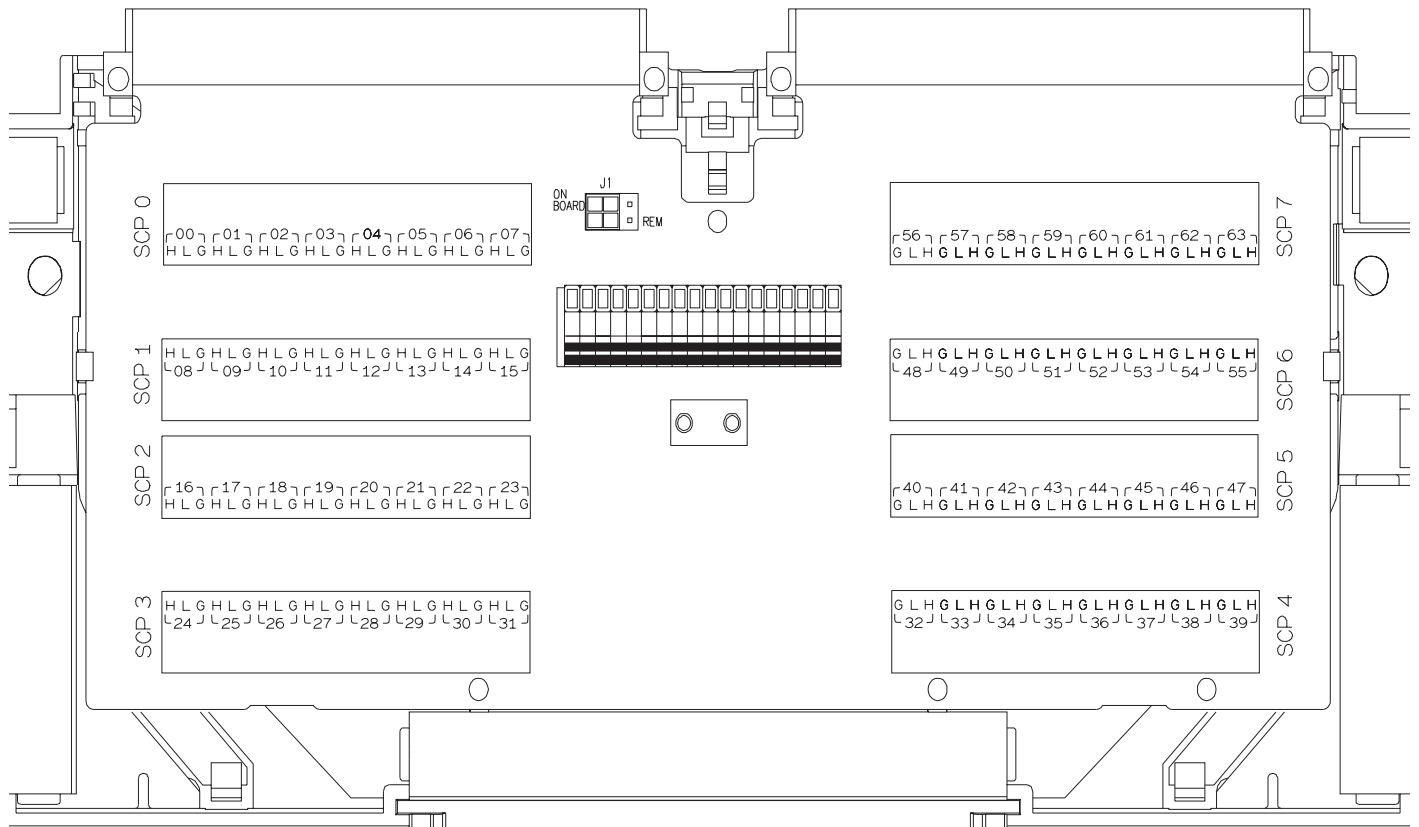



Figure 1. VT1512A C-Size Terminal Module Connections

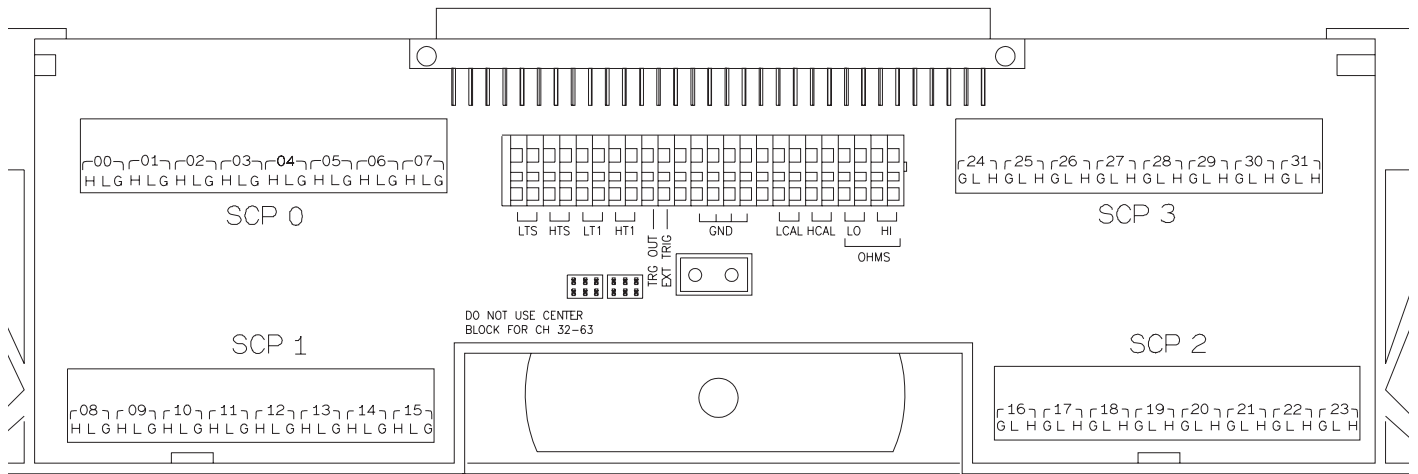

**Figure 2. VT1512A B-size Terminal Module Connections (Ch 00-31)**

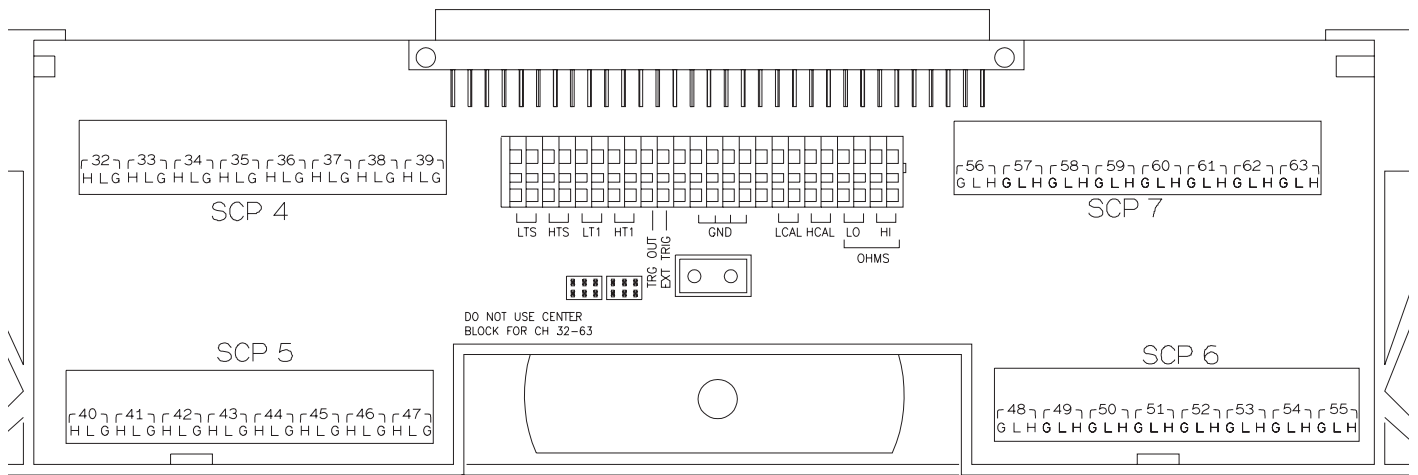

**Figure 3. VT1512A B-size Terminal Module Connections (Ch 32-63)**

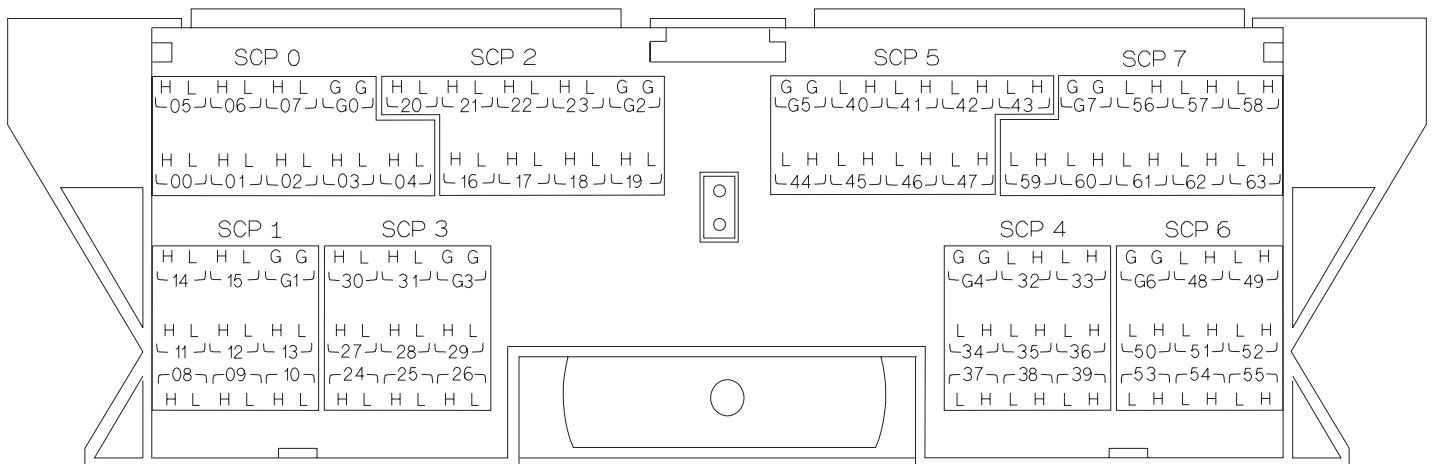

**Figure 4. Agilent/HP E1413 Option 12 Terminal Module Connections**

# Programming With SCPI Commands

The SCPI commands shown here are covered in Chapters 3 and 5 of your VT1413C or Agilent/HP E1313 manual. This section will relate those commands to the parameter values which are specific to this Plug-on.

**Checking the ID of the SCP** To verify the SCP type(s) installed on the VT1413C or Agilent/HP E1313 use the `SYSTem:CTYPe? (@<channel>)` command.

- The *channel* parameter specifies a single channel in the channel range covered by the SCP of interest. The first channel number for each of the eight SCP positions are; 0,8,16,24,32,40,48 and 56.

The value returned for the SCP in an Agilent/HP E1413B is:  
HEWLETT-PACKARD,E1413 Opt 12 8-Channel Fixed Filter SCP,0,0

The returned value for the SCP in a VT1413C or an Agilent/HP E1313 is:  
HEWLETT-PACKARD,E1512 8-Channel Fixed Filter SCP,0,0

To determine the type of SCP installed on channels 0 through 7 send

```
SYST:CTYP? (@100)           query SCP type @ ch 0
enter statement here
```

**Querying the Filter Cutoff Frequency** While the Low Pass Filter SCP does not provide programmable cutoff frequency the filter frequency can be queried. The response to this query will always be 25. To query any channel for its cutoff frequency use the `INPut:FILTer[:LPASs]:FREQuency? (@<channel>)` command. The `INP:FILT:FREQ?` command returns the numeric cutoff value currently set for the channel specified.

- The *channel* parameter must specify a single channel.

To query the cutoff frequency of channel 6 send

```
INP:FILT:FREQ? (@106)       query channel 6
enter statement here
```

**Querying the Filter State** While the Low Pass Filter SCP does not allow controlling whether the filters are enabled or disabled, this state can be queried. The response to this query will always be 1. To query any channel to determine if it is enabled or disabled use the `INPut:FILTer[:LPASs][:STATe]? (@<channel>)` command. The `INP:FILT?` command returns a 0 if the channel is OFF or a 1 if the channel is ON.

- The *channel* parameter must specify a single channel.

To query the filter state of channel 2 send

```
INP:FILT? (@102) query channel 2  
enter statement here
```

## Querying the Channel Gain

While the Low Pass Filter SCP does not provide amplifiers, the channel gain can be queried. The response to this query will always be 1. To query any channel to determine its gain setting use the `INPut:GAIN? (@<channel>)` command. The `INP:GAIN?` command returns the current gain value for the specified channel.

- The channel parameter must specify a single channel.

To query the gain setting of channel 8 send

```
INP:GAIN? (@108) query channel 8  
enter statement here
```

## Detecting Open Transducers

This SCP provides a method to detect open transducers. When Open Transducer Detect (OTD) is enabled, the SCP injects a small current into the HIGH and LOW input of each channel. The polarity of the current pulls the HIGH inputs toward +17 volts and the LOW inputs towards -17 volts. If a transducer is open, measuring that channel will return an over-voltage condition. OTD is available on a per SCP basic. all eight channels of an SCP are enabled or disabled together. See Figure 5 for a simplified schematic diagram of the OTD circuit.

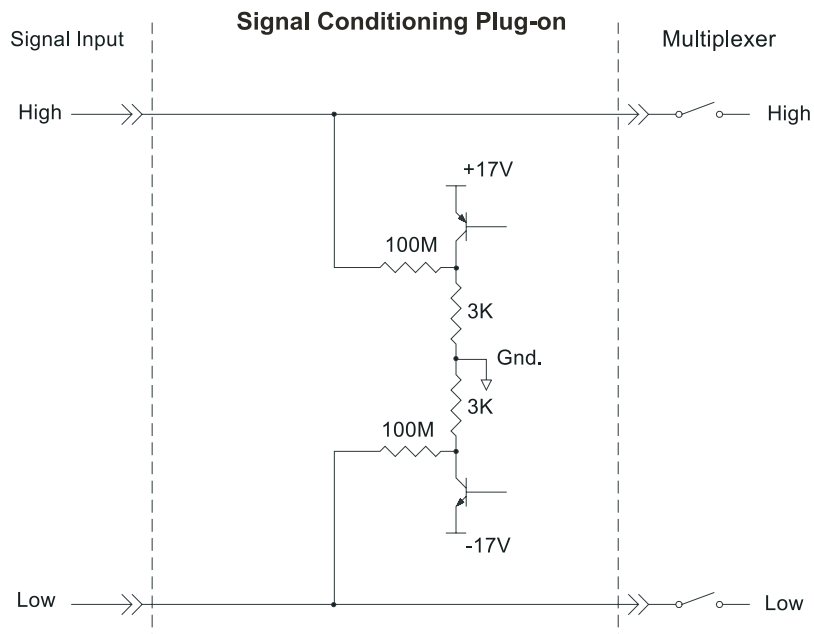


Figure 5. Open Transducer Detect Circuit

---

**NOTES** 1) When OTD is enabled, the inputs have up to 0.2  $\mu$ A injected into them. If this current will adversely affect your measurement, but you still want to check for open transducers, you can enable OTD, make a single scan, check the CVT for bad measurements, then disable OTD and make your regular measurement scans. The specifications apply only when OTD is off.

2) Allow 5 minutes before checking for open transducers to allow filter capacitors to charge.

---

To enable or disable Open Transducer Detection, use the **DIAGnostic:OTDetect** *<enable>*, (*@<ch\_list>*) command.

- The *enable* parameter can specify ON or OFF
- An SCP is addressed when the *ch\_list* parameter specifies a channel number contained on the SCP. The first channel on each SCP is:  
0, 8, 16, 24, 32, 40, 48 and 56

To enable Open Transducer Detection on all channels on SCPs 1 and 3:

DIAG:OTD ON, (@100,116) *0 is on SCP 1 and 16 is on SCP3*

To disable Open Transducer Detection on all channels on SCPs 1 and 3:

DIAG:OTD OFF, (@100,116)

## Register Based Programming

The register-based commands shown here are covered in Appendix D of the VT1413C or Agilent/HP E1313 manual. You should read that section first to become familiar with accessing registers and executing Register-Based Commands. This section will relate those commands to the parameter values which are specific to this Plug-on.

When Register Programming an SCP most communication is through the Signal Conditioning Bus. For that you will use the Register Commands:

SCBWRITE *<regaddr>* *<regvalue>*  
and  
SCBREAD? *<regaddr>*



### VT1512A Register Map

Read (returned value)	Write( <regvalue>)	SCP Register	<regaddr> Value
SCP ID (8040 <sub>16</sub> )		Whole SCP Reg 0	00ppp000000 <sub>2</sub>

ppp=Plug-on  
ccc=SCP channel

In addition you will access bits in the Card Control register to control Open Transducer Detection.

**Checking ID of SCP** To query an SCP for its ID value, write the following value to Parameter Register 1:  
 $(SCP\ number) \times 40_{16}$   
 Then write the opcode for SCBREAD? (0800<sub>16</sub>) to the Command Register. The ID value will be written to the Query Response Register.

**Detecting Open Transducers** Open Transducer Detection (OTD) is controlled by bits in the Card Control Register. For more information on OTD see Figure 1.

#### Card Control Register (Base + 12<sub>16</sub>)

15	14	14-13	12	11	10-8	7-0
PSI Pwr Reset	FIFO Mode	unused	FIFO Clear	VPPEN	A24 Window	Open Transducer Detect

Writing a one (1) to a bit enables open transducer detect on that signal conditioning module. Writing a zero (0) to a bit disables open transducer detect.

Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0
SCP 7	SCP 6	SCP 5	SCP 4	SCP 3	SCP 2	SCP 1	SCP 0

# Specifications

These specifications for the VT1512A reflect the combined performance of the VT1413C, Agilent/HP E1313 and the VT1512A Signal Conditioning Plug-on. These specifications are not to be added to those presented in the VT1413C and Agilent/HP E1313 User's Manuals.

## General Specifications

---

### Measurement ranges

DC Volts	±62.5 mV to ±16 V FS
Temperature	Thermocouples - -200 to +1700°C Thermistors - (VT1505A required) -80 to +160°C RTD's - (Opt 15 required) -200 to +850°C
Resistance	(Opt 15 required) 128 Ohms to 131 kOhms FS
Strain	25,000 $\mu\epsilon$ or limit of linear range of strain gage

---

**Maximum input voltage** Operating: <±16 V peak Damage level: >±42 V peak  
(Normal mode plus common mode)

---

**Maximum common mode voltage** Operating: <±16 V peak Damage level: >±42 V peak

---

**Normal mode rejection** @ 25 Hz -3 dB, @ 60 Hz > -20 dB

---

**Common mode rejection** 0 - 60 Hz -100 dB

---

**Input impedance** 100 MOhm±10% (each differential input to ground)

---

**Maximum tare cal offset** (Maximum tare offset depends on A/D range and SCP gain)

A/D range ±V F.Scale	16	4	1	0.25	0.0625
Max Offset	3.2213	0.82101	0.23061	0.07581	0.03792

**Measurement accuracy  
DC Volts**

(90 days) 23°C±1°C (with \*CAL? done after 1 hr warm up and CAL:ZERO? within 5 min.). If autoranging is ON, add ±0.02% FS to accuracy specifications.  
**For Agilent/HP E1313, multiply Noise Spec. by 1.4.**

Range ±V FS	Linearity % of reading	Offset Error	Noise 3 sigma	Noise* 3 sigma
0.0625	0.01%	7.2 μV	34 μV	15 μV
0.25	0.01%	12.2 μV	60 μV	28 μV
1	0.01%	33 μV	110 μV	92 μV
4	0.01%	122 μV	450 μV	366 μV
16	0.01%	488 μV	1.8 mV	1.5 mV

\* [SENSE:]FILTEr[:LPASs][:STATe] ON (max scan rate - 100 readings/s/channel)

Temperature Coefficients: Gain - 10ppm/°C. Offset - (0 - 30°C) no additional error, (30 - 40°C) 0.1 μV/°C,  
(40 - 55°C) 2.4 μV+0.27 μV/°C

**Measurement accuracy  
Temperature**

(90 days) 23°C±1°C (with \*CAL? done after 1 hr warm up and CAL:ZERO? within 5 min.). If autoranging is ON, add ±0.02% FS to accuracy specifications.

(simplified specifications, see temperature accuracy graphs in VT1413C manual for details)

The temperature accuracy specifications include instrument and firmware linearization errors. The linearization algorithm used is based on the IPTS-68(78) standard transducer curves. Add your transducer accuracy to determine total measurement error.

**Thermocouples**

<b>Type E</b>	A/D Filter	-200 to 0°C	0 to 200°C	200 to 400°C	400 to 800°C
	OFF ON*	2.25°C 1.65°C	0.65°C 0.34°C	0.50°C 0.24°C	0.45°C 0.23°C
<b>Type EExtended</b>	A/D Filter	-200 to 0°C	0 to 200°C	200 to 600°C	600 to 800°C
	OFF ON*	14.7°C 13.8°C	0.80°C 0.49°C	0.50°C 0.30°C	0.80°C 0.45°C
<b>Type J</b>	A/D Filter	-200 to 0°C	0 to 200°C	200 to 600°C	600 to 775°C
	OFF ON*	2.65°C 2.00°C	0.75°C 0.38°C	0.63°C 0.32°C	0.63°C 0.32°C
<b>Type K</b>	A/D Filter	-200 to 0°C	0 to 400°C	400 to 800°C	800 to 1400°C
	OFF ON*	4.30°C 3.35°C	0.90°C 0.50°C	0.85°C 0.40°C	1.10°C 0.52°C
<b>Type R</b>	A/D Filter	0 to 100°C	100 to 200°C	200 to 600°C	600 to 1000°C
	OFF ON*	6.90°C 3.80°C	5.00°C 2.60°C	4.00°C 1.95°C	3.10°C 1.70°C

\* [SENSE:]FILTEr[:LPASs][:STATe] ON (max scan rate - 100 readings/s/channel)

**Measurement accuracy  
Temperature (cont.)**

(simplified specifications, see temperature accuracy graphs in VT1413C or Agilent/HP E1313 manual for details)

**Thermocouples (cont.)**

Type S	A/D Filter	0 to 100°C	100 to 200°C	200 to 800°C	800 to 1750°C
	OFF	8.00°C	5.60°C	4.45°C	3.30°C
	ON*	5.20°C	3.25°C	2.40°C	1.60°C

Type T	A/D Filter	-200 to -100°C	-100 to 0°C	0 to 200°C	200 to 400°C
	OFF	3.40°C	1.90°C	0.90°C	0.70°C
	ON*	2.25°C	0.78°C	0.46°C	0.33°C

**5 kΩ Reference Thermistor**

A/D Filter	-10 to 65°C	65 to 85°C
OFF	0.011°C	0.021°C
ON*	0.0095°C	0.0115°C

**100 Ω Reference RTD**

A/D Filter	-125 to 75°C
OFF	0.75°C
ON*	0.36°C

**100 Ω RTD**

A/D Filter	-200 to 75°C	75 to 300°C	300 to 600°C	600 to 970°C
OFF	0.19°C	0.37°C	0.43°C	0.53°C
ON*	0.11°C	0.21°C	0.36°C	0.46°C

**2252 Ω Thermistor**

A/D Filter	0 to 30°C	30 to 70°C	70 to 80°C	80 to 100°C
OFF	0.012°C	0.013°C	0.014°C	0.024°C
ON*	0.010°C	0.012°C	0.010°C	0.014°C

**5 kΩ Thermistor**

A/D Filter	0 to 30°C	30 to 70°C	70 to 85°C
OFF	0.014°C	0.027°C	0.048°C
ON*	0.011°C	0.017°C	0.027°C

**10 kΩ Thermistor**

A/D Filter	0 to 30°C	30 to 60°C	60 to 90°C	90 to 115°C
OFF	0.015°C	0.024°C	0.034°C	0.059°C
ON*	0.013°C	0.016°C	0.021°C	0.032°C