

1. Checking the Parts in the Kit


Confirm that all parts listed below are included in the kit. If any part is shorted or any abnormality is found in the appearance of the parts, contact our sales representative where you bought the instrument.

List of parts included in the kit.

right side bracket (1pc), left side bracket (1pc), screws (M4, 12 mm long) (4pcs)

2. Joining the Instruments with Mounting Hardware

1. Turn handle (a) toward the rear of the instrument as shown in the figure below.
2. Remove sealing label (b) from the left and right sides of the instrument (4 labels).
3. If the four feet on the bottom of the instrument are covered with rubber stoppers, remove all of them.
4. Insert the projection in the left side bracket (c) into the slit in the ventilation hole on the left side of the instrument, then attach the left side bracket (c) with two M4 x 12 mm frame attachment screws (d).
Reference torque value: 1.4 to 1.5 N·m
5. Insert the projection in the right side bracket (e) into the slit in the ventilation hole on the right side of the instrument, then attach the right side bracket (e) with two M4 x 12 mm frame attachment screws (f).
Reference torque value: 1.4 to 1.5 N·m

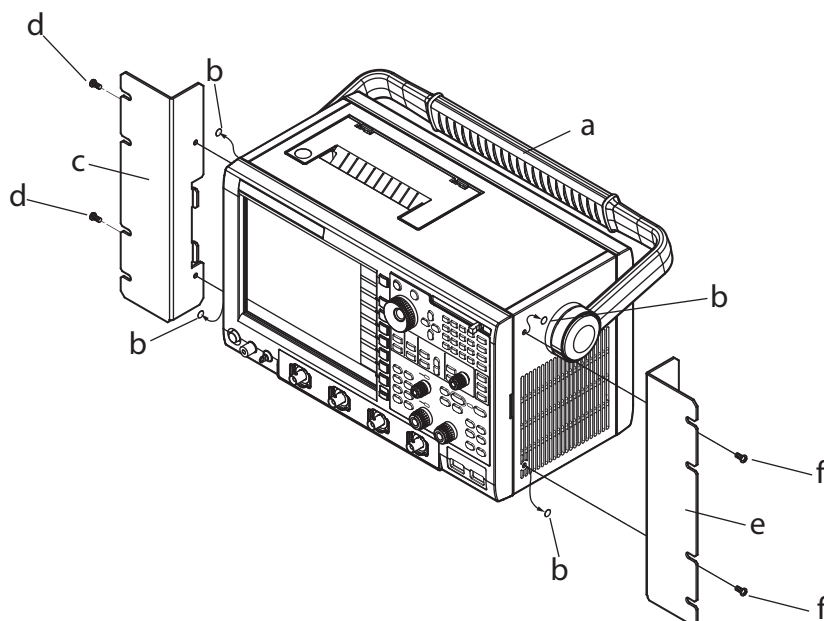

3. Mounting the Joined Instruments to the Rack

Dimensions after mounting to the rack are illustrated below.

Note:

1. Be sure to support the instrument from the bottom. When doing so, make sure not to cover the ventilation holes on the bottom of the instrument.
2. Provide a clearance of at least 100 mm around the instrument to prevent the temperature rise inside the instrument.

