
Foreword

This user's manual contains useful information about the precautions, functions, and operating procedures of the X-Wirepuller program that is downloadable from <http://www.yokogawa.com/tm/tm/softdownload.htm>. To ensure correct use, please read this manual thoroughly during operation.

After reading the manual, keep it in a convenient location for quick reference whenever a question arises during operation.

For information about the handling precautions, functions, and operating procedures of the DL series digital oscilloscopes, and the handling and operating procedures of Windows, see the manuals that accompany the particular instrument you are using.

Notes

- The contents of this manual are subject to change without prior notice as a result of continuing improvements to the instrument's performance and functions. The figures given in this manual may differ from the actual screen.
- Every effort has been made in the preparation of this manual to ensure the accuracy of its contents. However, should you have any questions or find any errors, please contact your nearest YOKOGAWA dealer.

Trademarks

- MS-DOS, Windows, and Windows NT are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.
- Adobe and Acrobat are trademarks of Adobe Systems incorporated.
- For purposes of this manual, the TM and ® symbols do not accompany their respective trademark names or registered trademark names.
- Other company and product names are trademarks or registered trademarks of their respective companies.

Revisions

1st Edition: September 2005

Contents

Foreword.....	ii
Product Overview.....	4
Notes on Using the Software.....	7
Chapter 1. Connection	
1.1 Controlling the DL Series.....	8
1.2 Setting Configurations.....	9
1.3 Creating / Breaking up Connection.....	11
Chapter 2. Functions.....	12
Chapter 3. Control Window Operation.....	15
Chapter 4. Exiting the Application.....	17

Product Overview

Functions

Controlling the DL Series Digital Oscilloscopes

Enables the DL9000 series digital oscilloscopes to be controlled from your PC via the NIC, USB, or GP-IB interface. When the software program starts, the front panel image of the connected DL (control panel) appears on the monitor of your PC. Using a mouse, you can control the DL from your PC through operations that are similar to those for the front panel keys of the instrument.

Saving Screen Images

Saves the screen image data displayed on your PC in BMP format.

Selecting the Control Window Size

You can select the size of the control window that is displayed on your PC from the choices below. When the display resolution of the PC is small, the control window can be displayed reduced in size.

- Larger: Displays the screen image of the DL using the same number of pixels as the number of pixels of the entire screen of the connected instrument.
- Standard: Displays the screen image of the DL using 65% of the number of pixels of the entire screen of the connected instrument.
- Smaller: Displays the screen image of the DL using 50% of the number of pixels of the entire screen of the connected instrument.
- Full screen: Displays the screen image of the DL with a full-screen mode.

Selecting the Display Update Rate

You can select the display update rate of the DL screen image from the following. However, the actual display update rate may be slower than the specified update rate depending on the network transmission system or the amount of communication load.

“300milliseconds to 10 seconds”

Updating the Screen

The screen image of the DL can be forcibly updated. This is done when the display update rate is set to a low value or when the display update is paused.


Pausing Display Update Operation

Pauses the display update operation.

Pausing the display update operation improves the response of the software program such as when turning ON/OFF numerous items at once or when entering values from a keyboard.

Control Screen

For DL9000 Series Digital Oscilloscopes

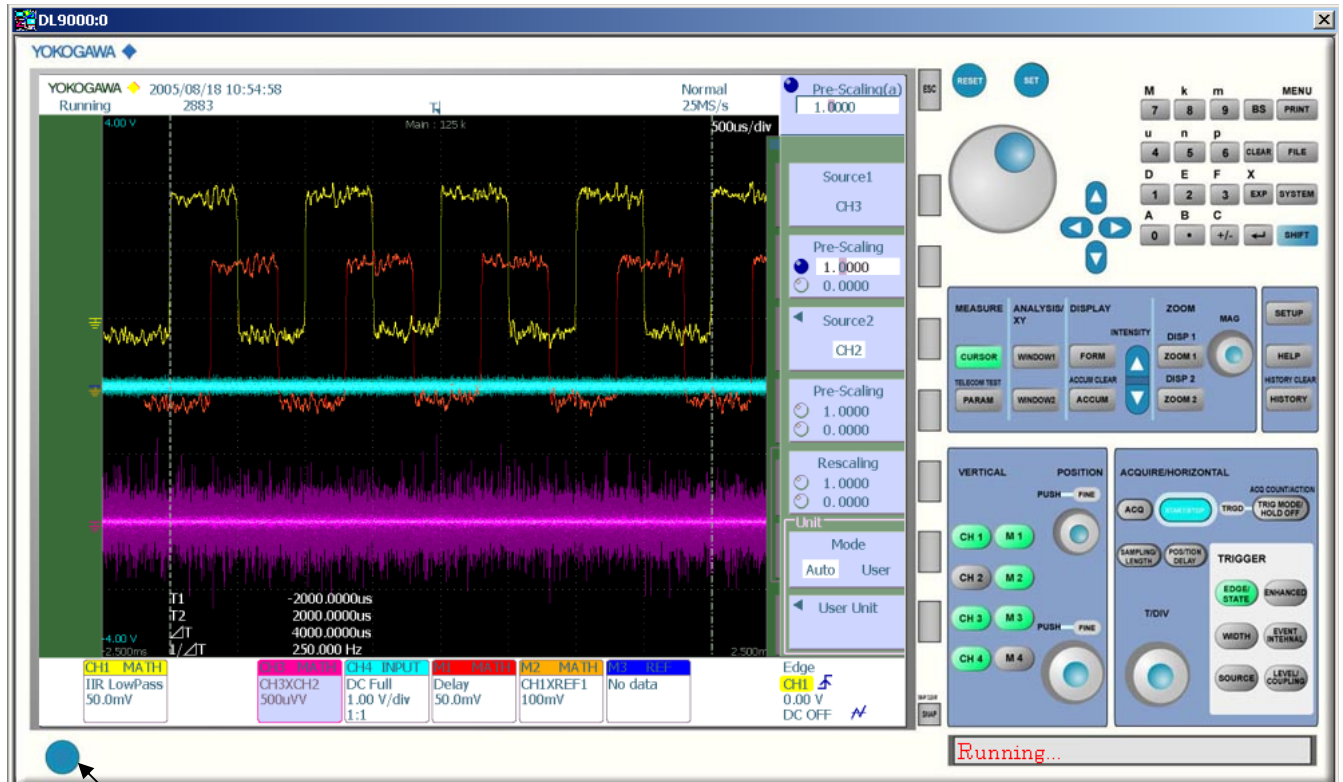

Break up connection to DL

PC System Requirements

PC

PC capable of running Windows 2000 and Windows XP with at least a Pentium 1 GHz processor and at least 256 MB of memory.

In addition, a USB driver for the connected DL is required. For details on the USB drivers, see the user's manual for the relevant DL.

CRT, printer, and mouse

Display: XGA or more

Color: 65536 colors or more

Must support Windows2000 and Windows XP.

GP-IB Board

When using the GP-IB interface, GP-IB board by National Instruments or a PCMCIA card is required.

DL Series Required for Operation

DL9000 Series: Version 1.60 or later

Notes on Using the Software

Exemption from Responsibility

Yokogawa Electric Corporation shall not be held responsible by any party for any losses or damage, direct or indirect, caused by the use or any unpredictable defect of the product.

Precautions Concerning the Use of the Software

- Do not perform operations directly on the DL series digital oscilloscopes while using this software program. Doing so can lead to erroneous operation.
- If the standby mode provided on your PC is activated, the operation of the software may not be able to continue.

When using the software, turn OFF the standby mode.


- If you run the software using a NIC interface, the line load is 1 Mbytes/s maximum. Consult your network administrator on using the NIC interface.
- If a connection error occurs when connecting to a DL digital oscilloscope, power cycle the DL.
- Do not set the network or communication parameters of the DL series using this software program. The connection may be disconnected.
- Do not execute self-tests using this software program.
- Simultaneous connections from multiple PCs to a single DL series digital oscilloscope are not allowed.

1.1 Controlling the DL Series

Setting the Interface

Set the interface to be used from the front panel of the DL.
For DL9000: SYSTEM > Remote Control > Device

- **Example (DL9140)**

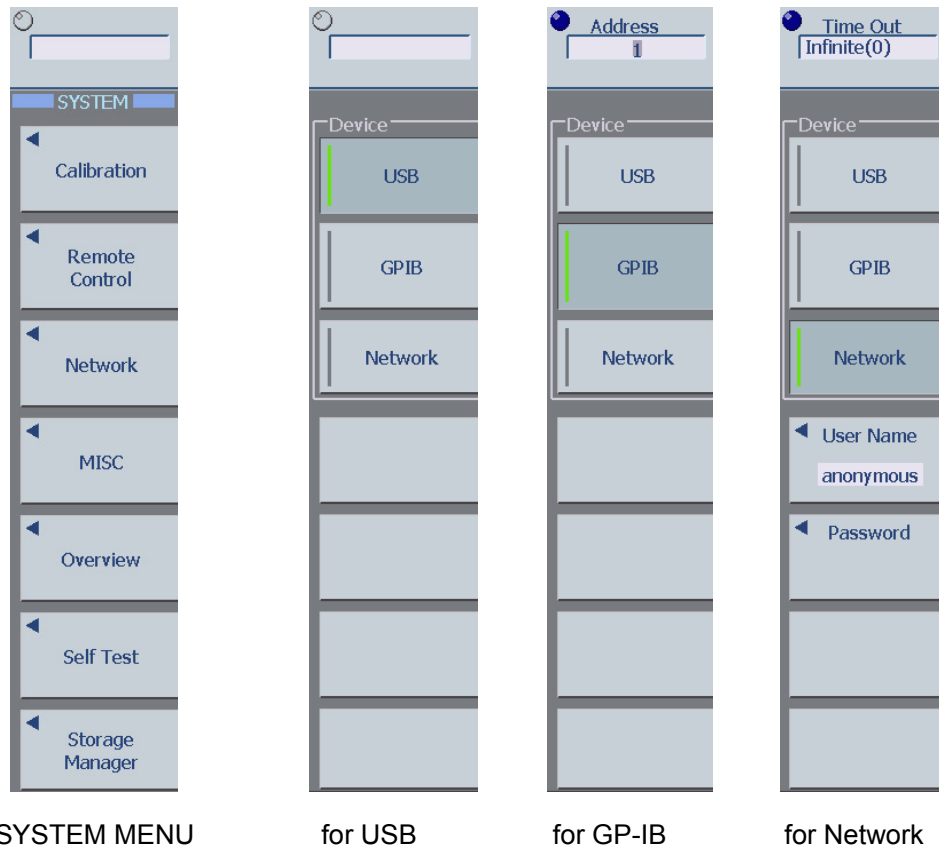


Note:

- For details on how to operate the DL, see the user's manual for the DL.
-

1.2 Controlling the DL Series


Click the file XWirepuller.exe to display the following window.

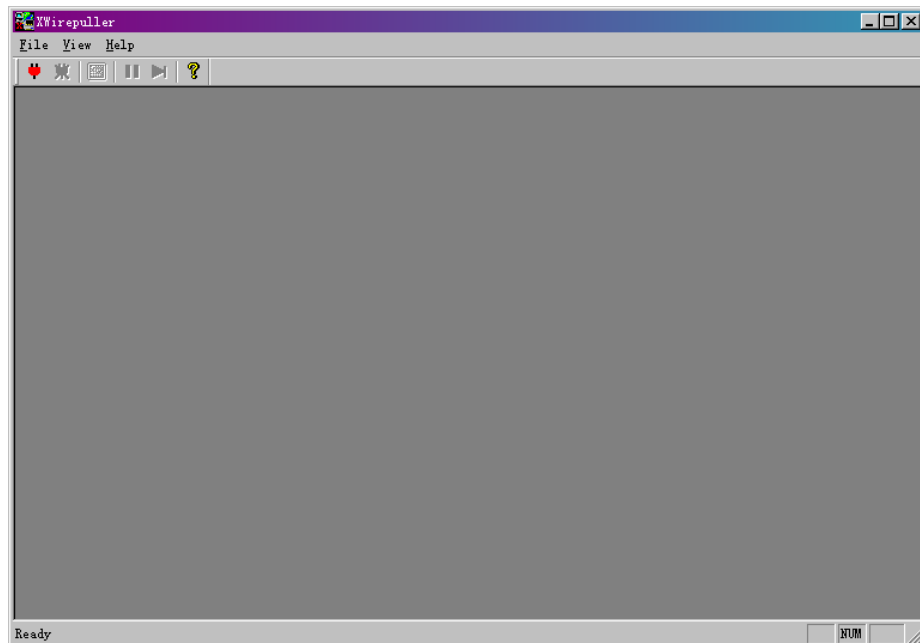


Note:

- Before creating communication with the DL, make sure that the cable between PC and DL has been correctly wired. For the hardware connection between PC and DL, please refer to the communication operation guide of your specific instrument.

Create Connection to the DL Instrument

Click **File > Connect** menu or  Icon, the connect dialog will then open. The predefined connection configurations are listed in it as follows.

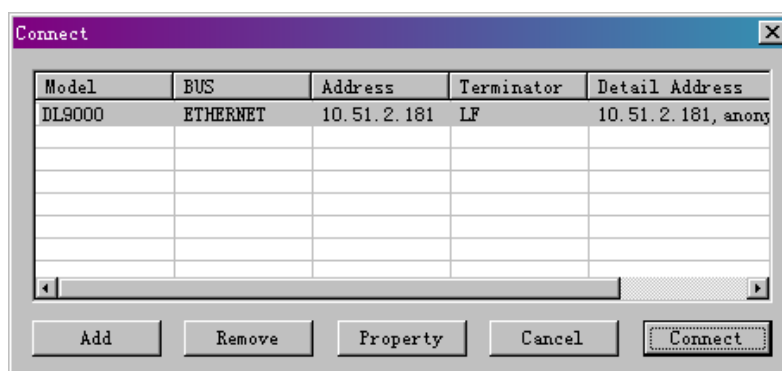


Add New Connection Configuration

The connection configuration list is empty at first start. To add new connection configuration to the DL, click the **Add** button. A new device configuration dialog will then open in which users can select the variable communication port and setup the corresponding parameters.

Set the interface to be used from the menu of the DL.

For DL9000: **SYSTEM > Remote Control**

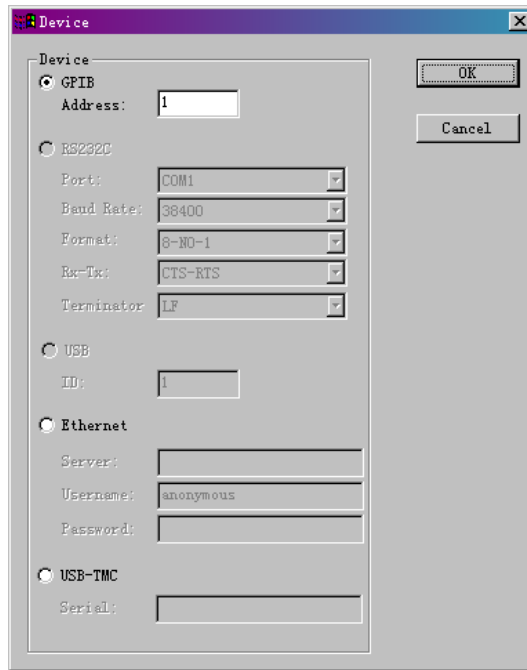

GPIB

Address: The unique ID of a GPIB device, ranges from 0~30

Ethernet

IP Address: The IP address or host name of the instrument
 Username: The login username for the **Remote Control** assigned by the instrument
 Password: The password for the username

USB-TMC

Serial: The serial No. of the instrument

Click the **OK** button to add new connection configuration into the configuration list. The program will try to check the correctness of the configuration, if succeeded, it will display the instrument model name, and otherwise it will return an error message and display "unknown" as model name.

Remove Connection Configuration

Click the **Remove** button to remove a selected connection configuration from the configuration list.


Change Connection Configuration's Parameters

Click the **Property** button to change a selected connection configuration's parameters, a configuration property setting dialog will then open which looks same as the new instrument dialog. Change the connection configuration's parameters and click the **OK** button to save changes.


1.3 Creating / Breaking up Connection

Create Connection to the DL Instrument

Select a defined connection configuration in the configuration list and click the **Connect** button to connect to the DL. (Double click on defined configuration in the list, also can create connection.) The program then will try to initialize the communication to the DL with selected configuration. If succeeded, the control window for the instrument will be displayed else, an error message will be displayed.

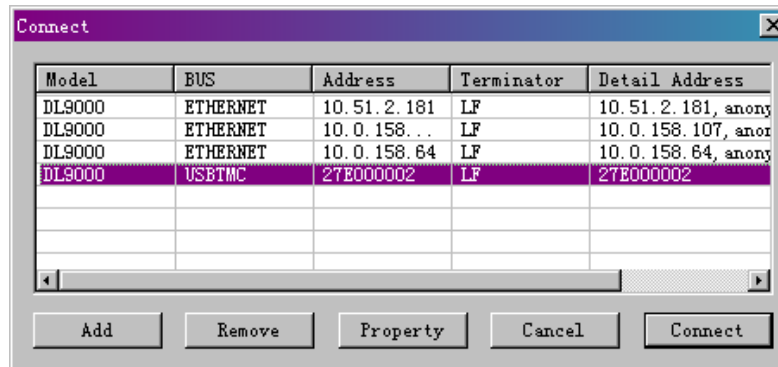


Break up Connection

Click **File > Disconnect** menu or  icon to break up current connection to the DL.

2. Functions

Operation panel


Click **View > Panel** menu to display or hide the operation panel.

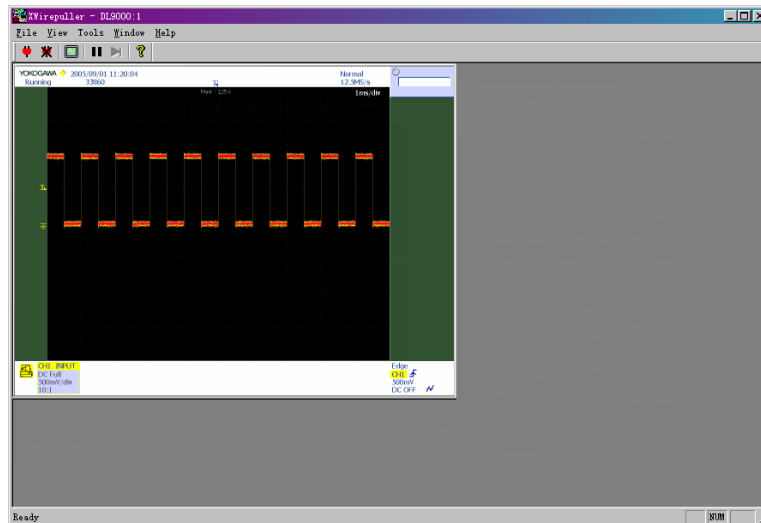


Control Window Size

Click **View > Zoom** menu to set the control window size.

- Larger: Displays the screen image of the DL using the same number of pixels as the number of pixels of the entire screen of the connected instrument.
- Standard: Displays the screen image of the DL using 65% of the number of pixels of the entire screen of the connected instrument.
- Smaller: Displays the screen image of the DL using 50% of the number of pixels of the entire screen of the connected instrument.

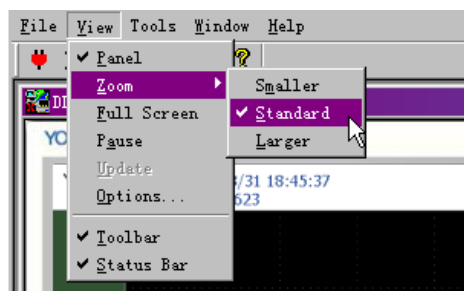

Full screen display


Click **View > Full Screen** menu or  icon to display with a full-screen mode. The full-screen mode ends if the “ESC” key of the personal computer is pushed, and it returns to a usual display.

The full-screen mode or display of the operation panel can be ended by pushing mouse's right button while pushing the “CTRL” key to the personal computer.

Updating the Screen

Click **View > Update** menu or  icon to update the screen image.


Pausing Display Update Operation

Click **View > Pause** menu or  icon to pause the display update operation.

Display update Interval


Click **View > Options** menu, the option dialog will open as follows.

The setting ranges of the interval are from 300 milliseconds to 10 seconds.

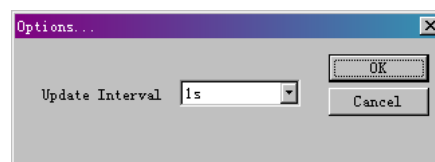

Saving Screen Images


Click **Tools > Image** menu to save the screen image data displayed on your PC in BMP format.

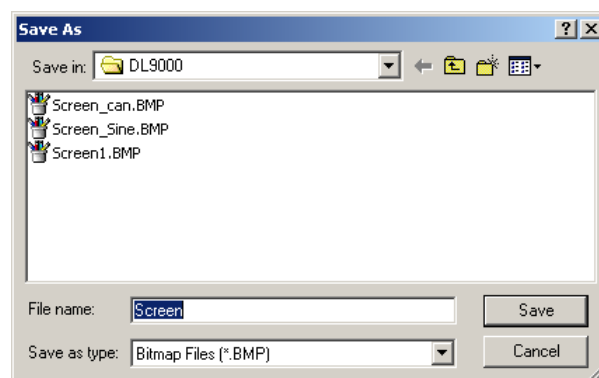

Two or more DL

Click **Window > Cascade** menu, all open windows are cascaded.

Moreover, the list of connected DL is displayed in the menu, and the window can be displayed on the foremost side by clicking it.

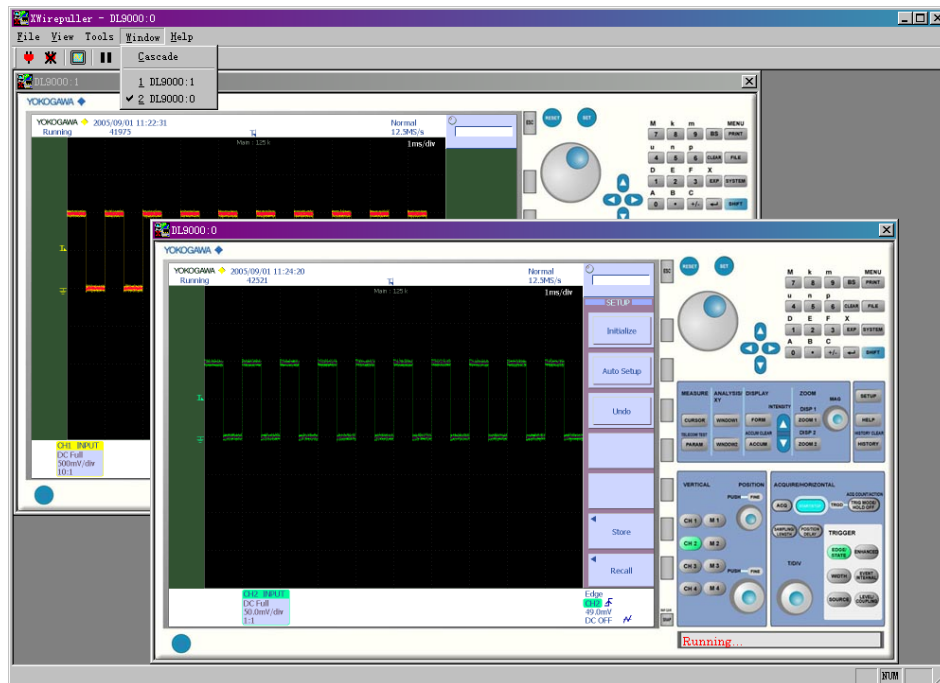

Note:

- When two or more DL is controlled, the connection might be cut by the situation connected DL and line. Please use it by the number that can be connected with stab










Viewing version information

Click the **Help** menu, the version of XWirepuller you are currently using is displayed.

3 Control Window Operation

Using the Mouse


The displayed icon and the mouse operation vary depending on where the mouse pointer is located on the control window. The following table shows the mouse operation for each icon and the operation of the DL series digital oscilloscopes.

Mouse Pointer Position	Displayed Icon and Mouse Operation	Operation
Operation key	 Click operation	Same as pressing the operation key
Screen	 Click operation Wheel operation	Same as the mouse operation of the DL series Same as the mouse operation of the DL series
Area to the left or right of the jog shuttle	 Click operation Wheel operation	Same as turning the jog shuttle to the left or right Same as turning the jog shuttle
Area to the left, right or center of the VERTICAL SCALE knob	 Click operation Wheel operation  Click operation	Same as turning the SCALE knob to the left or right Same as turning the SCALE knob Same as pressing the SCALE knob
Area to the left, right or center of the VERTICAL POSITION knob	 Click operation Wheel operation  Click operation	Same as turning the POSITION knob to the left or right Same as turning the POSITION knob Same as pressing the POSITION knob
Area to the left or right of the T/DIV knob	 Click operation Wheel operation	Same as turning the T/DIV knob to the left or right Same as turning the T/DIV knob
Area to the left or right of the MAG knob	 Click operation Wheel operation	Same as turning the MAG knob to the left or right Same as turning the MAG knob

Example of Mouse Operation


1. Operation Key Operation

Click to select Sine.

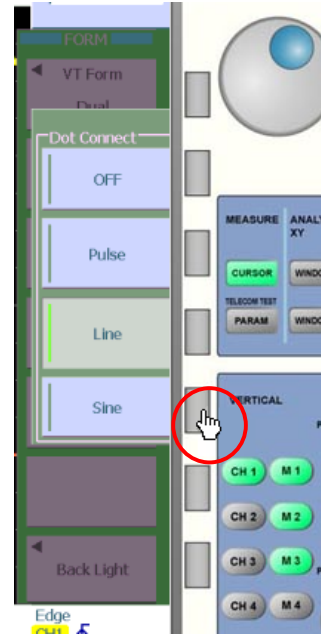

2. Jog Shuttle Operation

Click or operate the wheel to set.




3. VERTICAL POSITION Knob Operation

Push the knob to change FINE mode.



4. T/DIV Knob Operation

Turn the wheel to change the T/div setting.

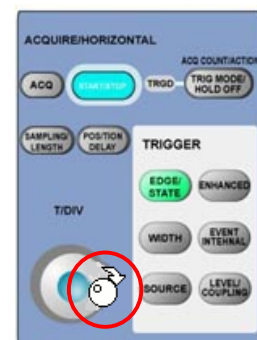

4 Exiting the Application

Exiting the Application

Click **File > Exit** menu or  icon to exit the application.