

---

**User's  
Manual**

**DL9040/DL9140/DL9240 Series  
Digital Oscilloscope  
Serial Bus Signal Analysis Function  
(I<sup>2</sup>C Bus Signal Analysis Function/CAN Bus Signal  
Analysis Function/SPI Bus Signal Analysis Function)**

---

---

Thank you for purchasing the DL9040/DL9140/DL9240 series Digital Oscilloscope with the Serial Bus Signal Analysis Function (option\*). This user's manual describes only the serial bus signal analysis function (I<sup>2</sup>C Bus Signal Analysis Function, CAN Bus Signal Analysis Function, and SPI Bus Signal Analysis Function). For information about other functions, operating procedures, and handling precautions of the DL9040/DL9140/DL9240 series, see the following manuals.

Manual Title	Manual No.	Description
DL9040/DL9140/DL9240 series User's Manual	IM 701310-01E	Explains all functions and procedures of the DL9040/DL9140/DL9240 series excluding the communication functions.
DL9040/DL9140/DL9240 series Communication Interface User's Manual (CD-ROM)	IM 701310-17E	Describes the communication interface functions.
* /F5 option:	Model with the I <sup>2</sup> C Bus Signal Analysis Function and SPI Bus Signal Analysis Function	
/F7 option:	Model with the CAN Bus Signal Analysis Function and SPI Bus Signal Analysis Function	
/F8 option:	Model with the I <sup>2</sup> C Bus Signal Analysis Function, CAN Bus Signal Analysis Function, and SPI Bus Signal Analysis Function	

## Notes

- The contents of this manual are subject to change without prior notice as a result of continuing improvements to the instrument's performance and functions. The figures given in this manual may differ from those that actually appear on your screen.
- Every effort has been made in the preparation of this manual to ensure the accuracy of its contents. However, should you have any questions or find any errors, please contact your nearest YOKOGAWA dealer as listed on the back cover of this manual.
- The contents of this manual may not be transcribed or reproduced, in part or in their entirety, without prior permission.

## Trademarks

- Microsoft, Internet Explorer, MS-DOS, Windows, Windows NT, and Windows XP are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.
- Adobe, Acrobat, and PostScript are trademarks of Adobe Systems Incorporated.
- For purposes of this manual, the TM and ® symbols do not accompany their respective trademark names or registered trademark names.
- Other company and product names are trademarks or registered trademarks of their respective holders.

## Revisions

- 1st Edition: September 2005
- 2nd Edition: March 2006

---

# Conventions Used in This Manual

## Safety Markings

The following markings are used in this manual.



*Improper handling or use can lead to injury to the user or damage to the instrument.* This symbol appears on the instrument to indicate that the user must refer to the user's manual for special instructions. The same symbol appears in the corresponding place in the user's manual to identify those instructions. In the manual, the symbol is used in conjunction with the word "WARNING" or "CAUTION."

---

**WARNING**

Calls attention to actions or conditions that could cause serious or fatal injury to the user, and precautions that can be taken to prevent such occurrences.

---

**CAUTION**

Calls attentions to actions or conditions that could cause light injury to the user or damage to the instrument or user's data, and precautions that can be taken to prevent such occurrences.

**Note**

Calls attention to information that is important for proper operation of the instrument.

## Notations Used on Pages Describing Operating Procedures

On pages that describe the operating procedures in Chapter 1 and 3, the following notations are used to distinguish the procedures from their explanations.

**Procedure**

This subsection contains the operating procedure used to carry out the function described in the current chapter. All procedures are written with inexperienced users in mind; experienced users may not need to carry out all the steps.

**Explanation**

This section describes the setup items and the limitations regarding the procedures.

## Notations Used in the Procedures

---

**Panel Keys and Soft keys**

Bold characters used in the procedural explanations indicate characters that are marked on the panel keys or the characters of the soft keys or menus displayed on the screen.

---

**SHIFT+Key**

*SHIFT+key* means you will press the SHIFT key to turn ON the SHIFT key followed by the operation key. The setup menu marked in purple above the panel key that you pressed appears on the screen.

---

**Rotary knob & SELECT**

Rotary knob & SELECT key indicates selecting or setting parameters and entering values using the rotary knob, the SET key, and other keys. For details on the procedure, see section 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.

---

## Unit

---

k Denotes 1000. Example: 100 kS/s

---

K Denotes 1024. Example: 459 KB (file data size)

---

# Contents

Conventions Used in This Manual .....	ii
<b>Chapter 1 I<sup>2</sup>C Bus Signal Analysis Function</b>	
1.1 Overview of the I <sup>2</sup> C Bus Signal Analysis Function .....	1-1
1.2 Setting the I <sup>2</sup> C Bus Signal Acquisition Conditions .....	1-2
1.3 Analyzing the Data .....	1-14
1.4 Searching the Waveform .....	1-20
1.5 Saving the Data of the Analysis Result List .....	1-25
1.6 Error Messages .....	1-30
<b>Chapter 2 CAN Bus Signal Analysis Function</b>	
2.1 Overview of the CAN Bus Signal Analysis Function .....	2-1
2.2 Setting the CAN Bus Signal Acquisition Conditions .....	2-3
2.3 Analyzing the Data .....	2-17
2.4 Searching the Waveform .....	2-25
2.5 Performing Stuff Bit Computation .....	2-29
2.6 Saving the Data of the Analysis Result List .....	2-32
2.7 Error Messages .....	2-33
<b>Chapter 3 SPI Bus Signal Analysis Function</b>	
3.1 Overview of the SPI Bus Signal Analysis Function .....	3-1
3.2 Setting the SPI Bus Signal Acquisition Conditions .....	3-3
3.3 Analyzing the Data .....	3-9
3.4 Searching the Waveform .....	3-17
3.5 Saving the Data of the Analysis Result List .....	3-22
3.6 Error Messages .....	3-23
<b>Chapter 4 Communication Commands</b>	
4.1 A List of Commands .....	4-1
4.2 ANALysis Group .....	4-15
4.3 MATH Group .....	4-22
4.4 SEARch Group .....	4-23
4.5 TRIGger Group .....	4-35
<b>Chapter 5 Specifications</b>	
5.1 I <sup>2</sup> C Bus Signal Analysis Function .....	5-1
5.2 CAN Bus Signal Analysis Function .....	5-2
5.3 SPI Bus Signal Analysis Function .....	5-3

## Index

1

2

3

4

5

Index

# 1.1 Overview of the I<sup>2</sup>C Bus Signal Analysis Function

## I<sup>2</sup>C Bus Signal Analysis Function

I<sup>2</sup>C Bus is an abbreviation for Integrated Circuit Bus. It is a bidirectional bus for connecting ICs. By using this function, you will be able to analyze data while displaying the I<sup>2</sup>C Bus signal waveform. The I<sup>2</sup>C Bus Signal Analysis Function consists of the following three main functions.


### Trigger Function <See page 1-2 for the operating procedure>

A trigger can be activated under the following conditions.

- When a start condition is detected.
- When a Nack is detected.
- When the specified address pattern (7-bit address, 7-bit address + sub address, or 10-bit address) is met.
- When the data pattern is met or not met.
- When a specified general call address is detected.


#### Address & Data Trigger Example

##### • When Activating a Trigger on the Start Condition or Address Pattern/Data Pattern

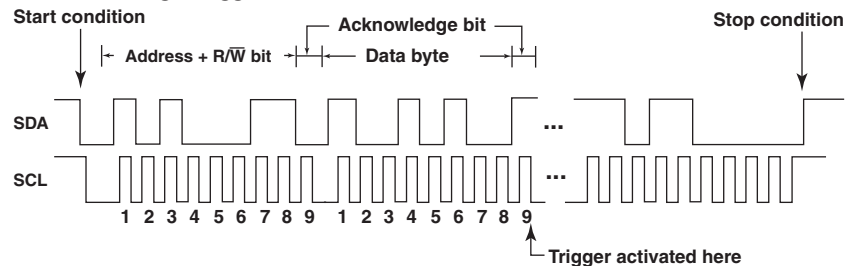

#### Nack Trigger Example

##### • When Activating a Trigger When the Acknowledge Bit Is Not Present (When the SDA Signal is high)

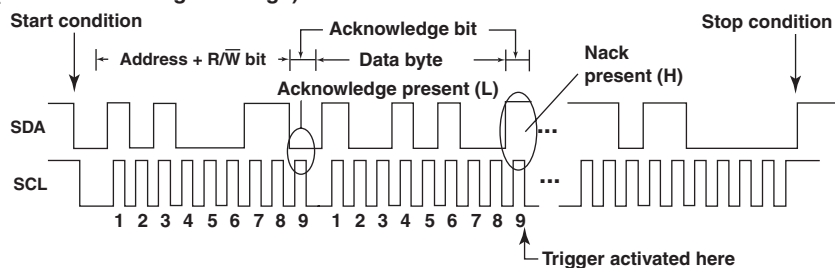

A trigger can be activated on the combination of the trigger conditions of the I<sup>2</sup>C bus signal and analog signal (event interval trigger). For details on the event interval trigger, see section 6.14 in the *User's Manual (IM701310-01E)*.

### Analysis Function <See pages 1-14 and 1-25 for the operating procedure>

This function analyzes the I<sup>2</sup>C bus signal data and shows a list of the analysis results. There are two types of analysis result lists: simple and detail. The simple list displays the analysis number, start and stop conditions, analysis data, address and data types, read/write signal, and the status of the Acknowledge bit for each byte. The detail list displays the time from the trigger position and data information in addition to the items displayed by the simple list. The data of the detail list can be saved to an arbitrary storage medium in CSV format. In addition, you can select an arbitrary byte in the analysis result list and move the zoom position (the center of the zoom box) to the head of that byte.

### Search Function <See page 1-20 for the operating procedure>


This function searches for data that matches a specific address pattern, data pattern, or Acknowledge bit status in the I<sup>2</sup>C bus signal data. When the search is executed, the zoom box (ZOOM1 or ZOOM2) moves to the data position where the conditions are met, and the data is displayed expanded in the zoom window.

## 1.2 Setting the I<sup>2</sup>C Bus Signal Acquisition Conditions

I<sup>2</sup>C Bus signal is acquired using a certain condition\* of the I<sup>2</sup>C Bus signal as a trigger condition.

\* When a start condition is detected, when a Nack is detected, when a specified address pattern is met, when a data pattern is met or not met, etc.

### Procedure




- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Trigger Conditions of the I<sup>2</sup>C Bus Signal

1. Press **ENHANCED** to display the ENHANCED menu.
2. Press the **Type** soft key to display the trigger type selection menu.
3. Press the **I<sup>2</sup>C** soft key.

### Selecting the Trigger Mode

4. Press the **Mode** soft key to display the trigger mode of the I<sup>2</sup>C bus signal selection menu.
5. Press any of the soft keys, **Every Start**, **ADR & DATA**, **NON ACK**, **General Call**, or **Start Byte/HS Mode** to set the trigger mode.

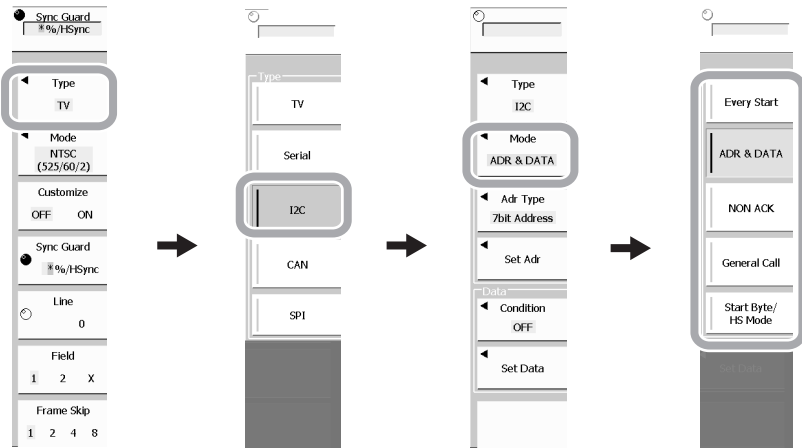

Proceed to the steps indicated below depending on the specified trigger mode.


- Every Start (trigger when the start condition is detected):  
The setting procedure is complete.
- ADR & DATA (trigger on an address pattern or data pattern): Step 6
- NON ACK (trigger when a Nack is detected): Step 21
- General Call (trigger on the general call address): Step 23
- Start Byte/HS Mode (trigger on the start byte or HS mode start condition): Step 27

• **Activating a Trigger on an Address Pattern/Data Pattern**


- After step 4 of page 1-2, Press the **ADR & DATA** soft key.

**Setting the Address Pattern**


- Press the **Adr Type** soft key to display the address type selection menu.
- Press the soft key corresponding to the desired address type.
- Press the **Set Adr** soft key. A screen for entering the address pattern appears. The screen varies depending on the specified address type.
- Turn the **rotary knob**, **arrow** keys, and **SET** key to set the pattern. You can use the soft keys to change the format to binary or hexadecimal or clear all the bits (X).
- Press **ESC**.

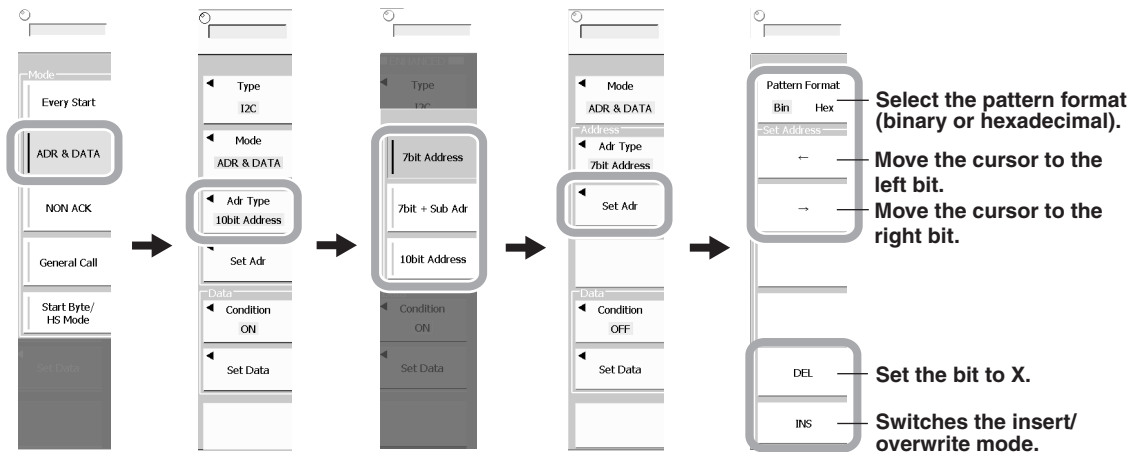


**7bit Address in Binary**

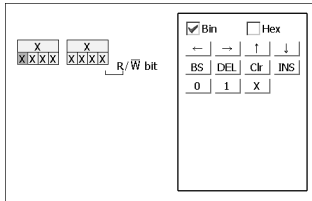


**7bit Address in Hexadecimal**

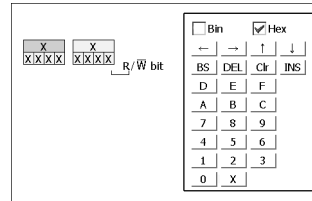


**7bit+Sub Address in Binary**

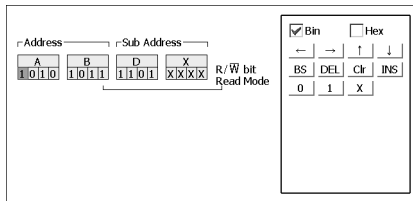


**7bit+Sub Address in Hexadecimal**

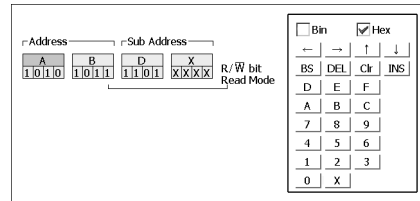

**10bit Address in Binary**

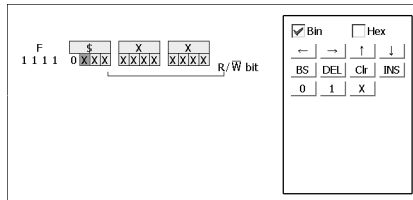


**10bit Address in Hexadecimal**

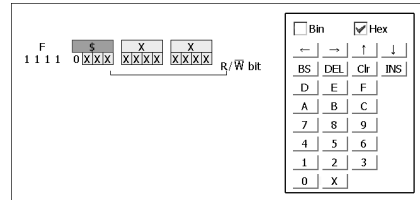

## 1.2 Setting the I<sup>2</sup>C Bus Signal Acquisition Conditions

### Setting the Data Pattern


12. Press the **Condition** soft key to display a data pattern setting menu.
13. Press the **Data** soft key to select ON (use a data pattern) or OFF (not use a data pattern). If you select ON, continue with the steps below. If you select OFF, you are done.
14. Press the **Condition** soft key to select True (activate a trigger when the data matches the specified data pattern) or False (activate a trigger when the data does not match the specified data pattern).
15. Press the **Pos Mode** soft key to select X (ignore) or Select.
16. If you select Select, use the **rotary knob** to specify the data position in the pattern to be compared.
17. Press any of the soft keys, **1 byte**, **2 byte**, **3 byte**, or **4 byte** to set the data size.
18. Press **ESC**.
19. Press the **Set Data** soft key to display a data pattern setting screen.
20. Turn the **rotary knob**, **arrow** keys, and **SET** key to set the pattern.  
You can use the soft keys to change the format to binary or hexadecimal, or clear all the bits (X).

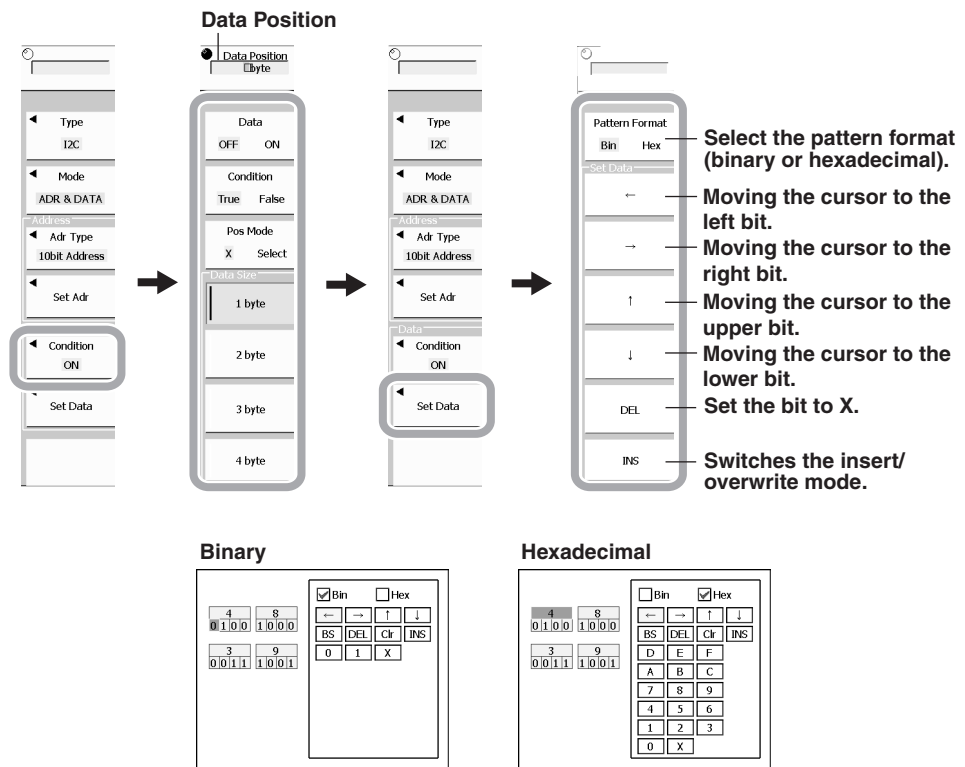




• **Activating a Trigger When a Nack Bit Is Detected**

21. After step 4 of page 1-2, press the **NON ACK** soft key.
22. Set whether to discard the Nack of Start Byte, HS Mode, and Read Access or include them in the trigger conditions.  
Press each of the **Start Byte**, **HS Mode**, and **Read Access** soft keys and select OFF (include in the trigger conditions) or ON (not include in the trigger conditions).

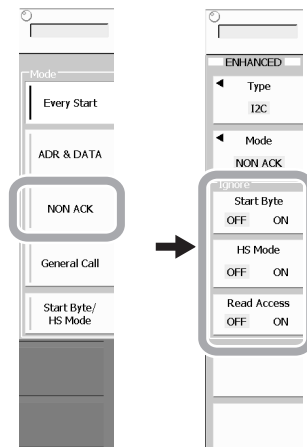

• **Activating Triggers on an General Call Data Pattern**


23. After step 4 of page 1-2, Press the **General Call** soft key.
24. Press the **Second Byte** soft key to display a menu used to select the format of the Second Byte.
25. Press a soft key corresponding to the desired Second Byte format.
  - When you select X, 0000 0100, or 0000 0110: The setting procedure is complete.
  - When you select 7bit Master Adr: Proceed to step 26.
26. Set the address pattern and data pattern in the same fashion as “Setting the Address Pattern” and “Setting the Data Pattern” in “Activating a Trigger on an Address Pattern or Data Pattern” of page 1-3.

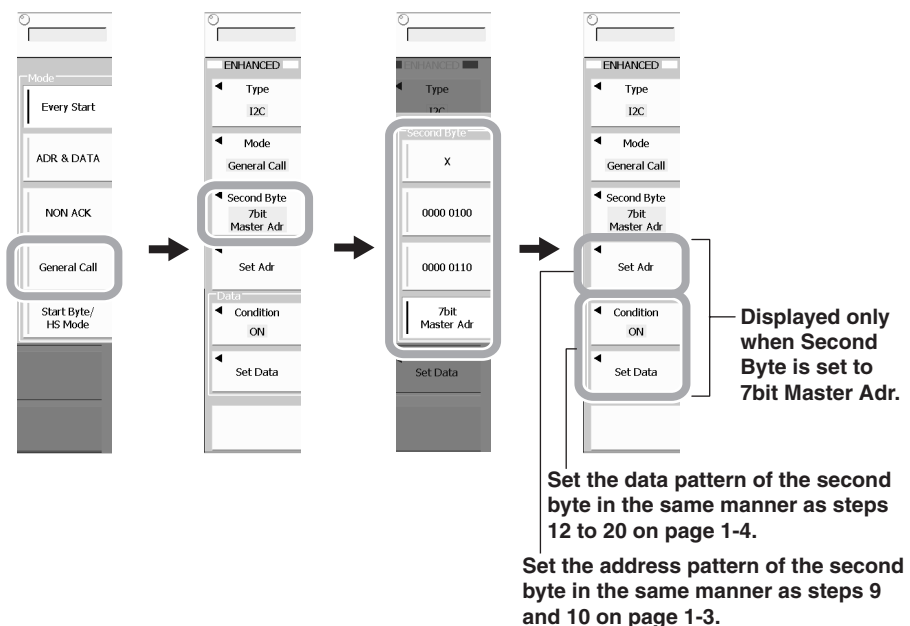

## 1.2 Setting the I<sup>2</sup>C Bus Signal Acquisition Conditions

- **Activating a Trigger on the Start Byte or HS Mode Start Condition**

27. After step 4 of page 1-2, Press the **Start Byte/HS Mode** soft key.
28. Press the **Start Byte** or **HS Mode** soft key to select whether to activate a trigger on the start byte or high speed mode start condition.

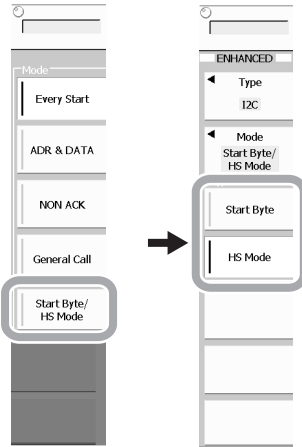

### Setting the Source Channel

29. Press **SOURCE** on the front panel to display the SOURCE menu.

#### Setting the SDA Signal

30. Press the **SDA** soft key to display a menu used to select a channel to be the SDA signal.
31. Press any of the soft keys **CH1** to **CH4** to assign the channel to be the SDA signal.

#### Setting the SCL Signal


32. Press the **SCL** soft key to display a menu used to select a channel to be the SCL signal.
33. Press any of the soft keys **CH1** to **CH4** to assign the channel to the SCL signal.

#### Setting the Qualification of the Channels Excluding the SDA Signal and SCL Signal

34. Press a channel soft key other than the channels set to the SDA or SCL signal to select H (high), L (low), or X (don't care). If H or L is selected, a trigger is activated on the logical OR or AND of the trigger conditions of the I<sup>2</sup>C bus signal and the trigger conditions of the channels other than the SDA or SCL signal.

#### Setting the Qualification Logic

35. Press the **Logic** soft key to select AND (logical product) or OR (logical sum).

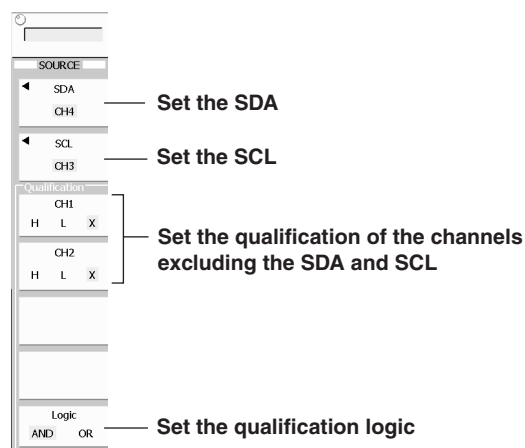

**Setting the Level, Coupling, HF Rejection, and Hysteresis**

36. Press **LEVEL/COUPLING** on the front panel to display the LEVEL/COUPLING menu.

**Selecting the Channel to Be Configured**

37. Press the **CH** soft key to display a channel selection menu.  
38. Press any of the soft keys, **CH1** to **CH4**.

**Setting the Level**

39. Turn the **rotary knob** to set the level used to determine high/low.

**Setting the Coupling**


40. Press the **Coupling** soft key to select DC.

**Setting the HF Rejection**

41. Press the **HF Rejection** soft key to display a HF rejection selection menu.  
42. Press any of the soft keys, **OFF**, **20MHz**, or **15kHz**.

**Setting the Hysteresis**

43. Press the **Hysteresis** soft key to select the hysteresis.

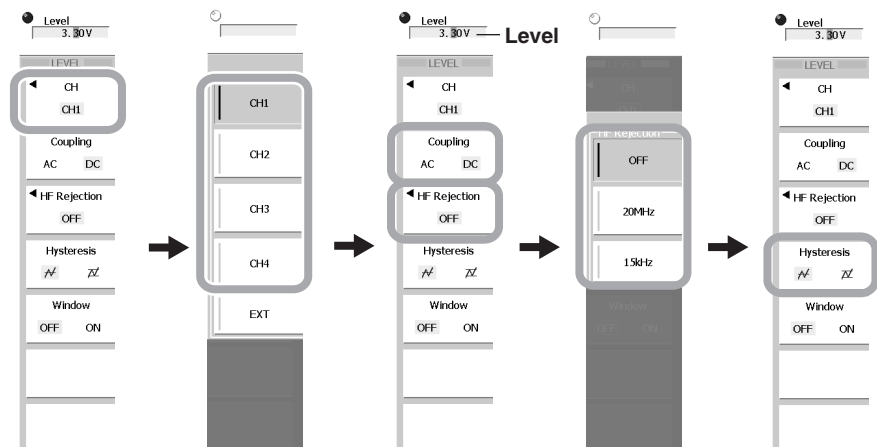

As necessary, repeat steps 37 to 43.

**Explanation****I<sup>2</sup>C Bus Signal Trigger Mode**

Select the trigger mode from the following list.

**Every Start**

Activate a trigger at the same time the start condition is detected

**ADR & DATA**

Activate a trigger on the address pattern or data pattern (Address & data trigger)

**NON ACK**

Activate a trigger when a Nack is detected (Nack trigger)

**General Call**

Activate a trigger on the general call address pattern


**Start Byte/HS Mode**

Activate a trigger on the start byte or high speed mode start condition

## 1.2 Setting the I<sup>2</sup>C Bus Signal Acquisition Conditions


- **Every Start**

When the start condition is detected, a trigger is activated on the falling edge of the SDA signal.

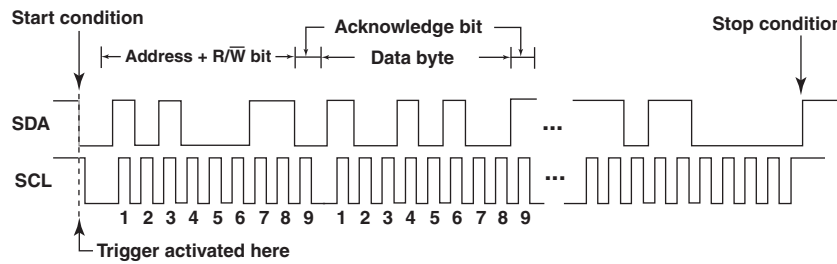

- **ADR & DATA (Address & Data Trigger)**

When the data matches the specified address pattern or data pattern, a trigger is activated on the falling edge of the acknowledge bit.

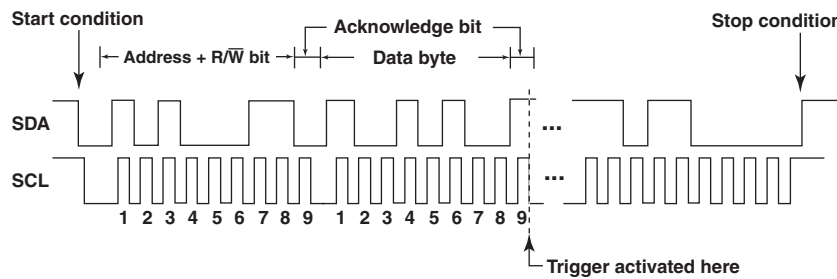

- **Address Type (Adr Type)**

Set the address type to 7-bit address, 7-bit + sub address, or 10-bit address.

- **Address (Set Adr)**

Set the pattern according to the address type. The data matching the specified pattern is one of the trigger conditions.

- **Data Condition**

To activate a trigger on a data pattern, set Data to ON in data conditions, and set the Condition, Pos Mode, Data Position, and Data Size items.

**Pattern Condition**

Select the pattern condition from below.

True	A trigger is activated when the data matches the data pattern.
False	A trigger is activated when the data does not match the data pattern.

**Position in the Pattern to Be Compared (Pos Mode, Data Position)**

Select the Pos Mode from below.

X	Does not use the position where the pattern is compared (Data Position) as a trigger condition.
Select	Set the position where the pattern is to be compared (Data Position) in terms of the number of data bytes. Set the data position in the range of 0 to 9999 bytes.

**Data Size**

Set the number of data bytes of the data pattern in the range of 1 to 4 bytes.

**Examples of setting**


This section will indicate the data sequence in bytes (hexadecimal notation) and indicate the position where the trigger will occur. The symbols used in the figures are as follows:

S: Start condition, P: Stop condition, Shaded area: Byte pattern to be compared.

• **Activating a Trigger Only on the Address Pattern**

**Trigger conditions**

Mode	ADR & DATA	
Address	Adr Type: Set Adr:	7bit Address 4A
Data	Data	OFF

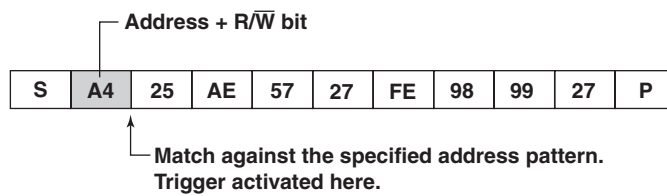


• **Activating a Trigger Only on the Data Pattern**


**Trigger conditions**

Mode	ADR & DATA	
Address	Set Adr	Not applicable
Data	Data Condition Data Size Set Data	ON True 2 bytes 27, AE

**<Data Position: X>**

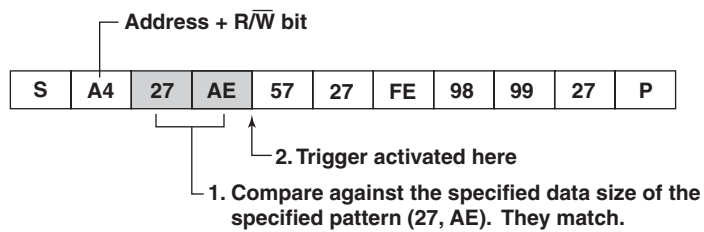

**<Data Position: 3>**

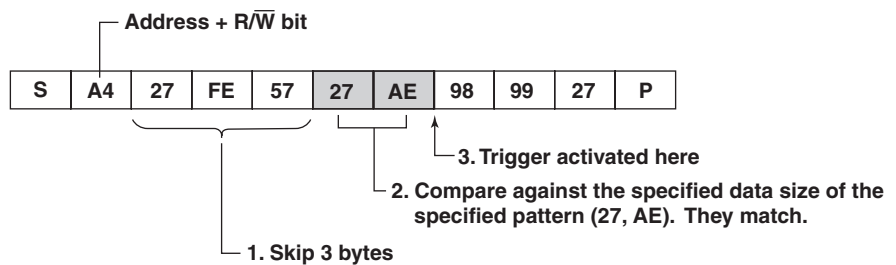


**1.2 Setting the I<sup>2</sup>C Bus Signal Acquisition Conditions**

• **NON ACK (Nack Trigger)**

**Activating a Trigger When the Acknowledge Bit Is High**

A trigger is activated when the Acknowledge bit is Nack (when the SDA signal is set to “H”).

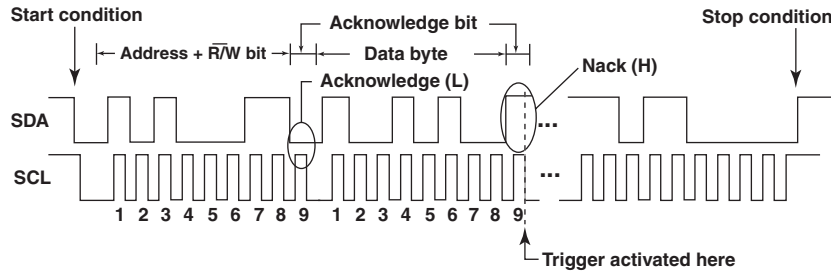


**Note**

You can select any of the Acknowledge bits, the status byte, HS mode master code, or read access byte, to be used for triggering.

• **General Call Trigger**

A trigger is activated on a general call address (Address: 0000 0000).

The second byte pattern after the general call address can also be used for triggering.

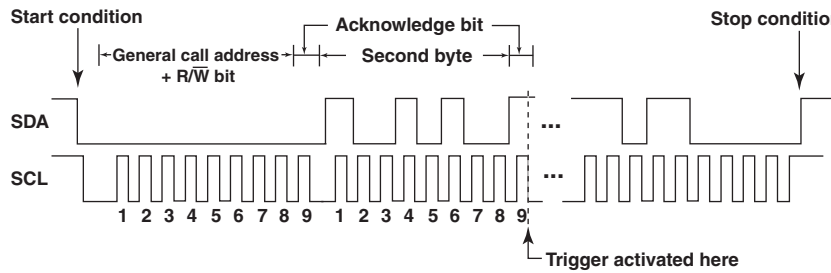

• **Second Byte**

Select the second byte from below.

X	Does not use the second byte pattern as a trigger condition.
0000 0100	Activates a trigger when the second byte pattern is 0000 0100.
0000 0110	Activates a trigger when the second byte pattern is 0000 0110.
7bit Master Adr	Arbitrarily set 7bit Master Adr of the second byte pattern.

**Examples of setting**


This section will indicate the data sequence in bytes (hexadecimal notation) and indicate the position where the trigger will occur. The symbols used in the figures are as follows:

S: Start condition, P: Stop condition, Shaded area: Byte pattern to be compared.

• **Activating a Trigger Only on the General Call Address**

**Trigger conditions**


Mode	General Call
Second Byte	Not applicable

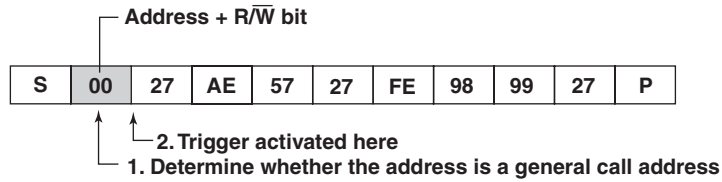

• **Activating a Trigger on the Second Byte Pattern Set to 06**

**Trigger conditions**

Mode	General Call
Second Byte	0000 0110

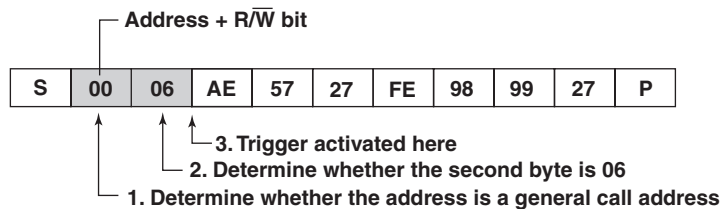


• **Activating a Trigger on an Arbitrary Pattern on the Second and Subsequent Bytes**


**Trigger conditions**

Mode	General Call	
Second Byte	7bit Master Adr (1010 1011)	
Data	Data	ON
	Condition	True
	Data Size	2 bytes
	Set Data	27, AE

<Data Position:X>

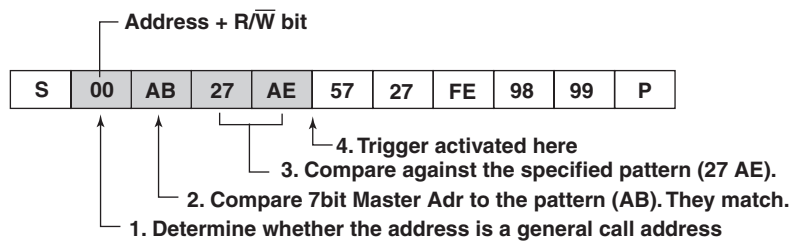

<Data Position:3>

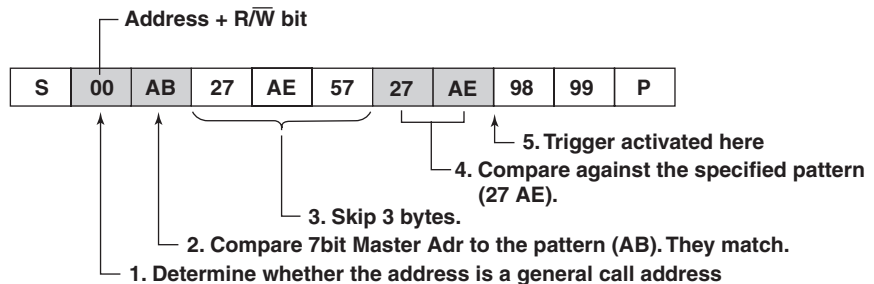


1.2 Setting the I<sup>2</sup>C Bus Signal Acquisition Conditions

• **Start Byte/HS Mode Trigger**

A trigger is activated on the start byte or HS mode master code.


• **Start Byte (Address: 0000 0001)**

When a start byte is detected, a trigger is activated.

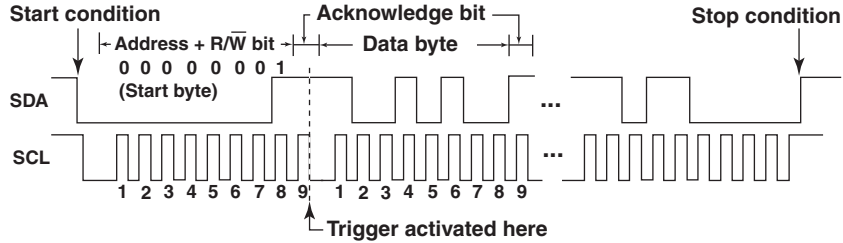

• **HS Mode**

A trigger is activated when the master code (Address: 0000 1xxx) of HS mode (high speed mode) is detected.

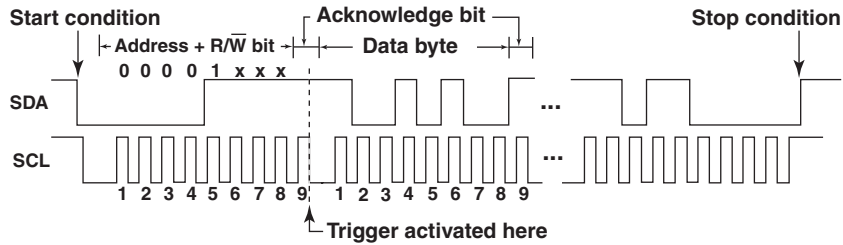

**Examples of setting**

This section will indicate the data sequence in bytes (hexadecimal notation) and indicate the position where the trigger will occur. The symbols used in the figures are as follows:

S: Start condition, P: Stop condition, Shaded area: Byte pattern to be compared.

• **Activating a Trigger Only on the Start Byte**

**Trigger conditions**

Mode	Start Byte/HS Mode
Type	Start Byte



**Source Channel**

The source channel of the I<sup>2</sup>C bus signal is set using the SOURCE menu that appears when you press the SOURCE key. The menu used to set the source channel of the I<sup>2</sup>C bus signal appears only when Type is set to I<sup>2</sup>C in the ENHANCED menu.

**Specifying the I<sup>2</sup>C Bus Signal (SDA and SCL Signals)**

The SDA and SCL signals are assigned to channels using the SOURCE menu.

**Trigger Conditions of the Channels Other Than I<sup>2</sup>C Bus Signal (Qualification)**

A trigger can be activated on the combination of the trigger conditions of the I<sup>2</sup>C bus signal (SDA/SCL signal) and the trigger conditions of the channels other than the I<sup>2</sup>C bus signal. Select the trigger conditions of the channels other than the I<sup>2</sup>C bus signal from the following:


- H The trigger source level is above the preset trigger level.
- L The trigger source level is below the preset trigger level.
- X Not used as a trigger source.



**Logic**

If the trigger condition of a channel other than the SDA or SCL signal is set to H or L, a trigger is activated on the trigger conditions of the I<sup>2</sup>C bus signal and the trigger conditions of the channels other than the SDA and SCL signals. Select the logic to used from the following:

- AND A trigger is activated when both the trigger conditions of the I<sup>2</sup>C bus signal and the trigger conditions of the channels other than the I<sup>2</sup>C bus signal are met.
- OR A trigger is activated when either the trigger conditions of the I<sup>2</sup>C bus signal or the trigger conditions of the channels other than the I<sup>2</sup>C bus signal are met.

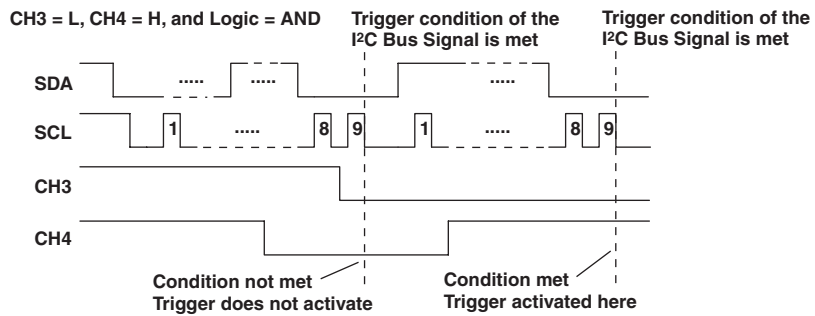

**Note**

To activate a trigger only on the SCL and SDA signals (trigger condition of the I<sup>2</sup>C bus), set the status of the other channels to ignore (X), and set the logic to AND.

**Trigger Level, Trigger Coupling, Etc.**

Set the trigger level, trigger coupling, HF rejection, and hysteresis of each channel. For details on these items, see the *User's Manual (IM701310-01E)*.

**Unification of the Trigger Setting of the I<sup>2</sup>C Bus Signal and the Setting of the I<sup>2</sup>C Bus Signal Analysis and Search**

On products with software version 1.80 or higher, the trigger settings of the I<sup>2</sup>C bus signal on the menu that is entered through the ENHANCED key and the settings of the I<sup>2</sup>C bus signal analysis and search on the menu entered through the WINDOW1 and ZOOM1 key are common. The CH1 to CH4 sources are the waveforms of which the settings are common.

**Trigger settings of the I<sup>2</sup>C bus signal that are applied to the settings of both the I<sup>2</sup>C bus signal analysis and search**

Level (trigger level), Hysteresis (trigger hysteresis)  
 (The settings of the I<sup>2</sup>C bus signal analysis and search are not applied to the trigger settings of the I<sup>2</sup>C bus signal.)

**Item of which the trigger settings of the I<sup>2</sup>C bus signal, the settings of the I<sup>2</sup>C bus signal analysis, and the settings of the I<sup>2</sup>C bus signal search that are mutually applied**

SDA Source, SCL Source


**Note**

- M1 to M4 are does not apply to the common settings.
- The settings of the I<sup>2</sup>C bus signal analysis and search on the menu entered through the WINDOW2 and ZOOM2 keys are not made common. They are independent settings.
- If you change common items (excluding Level and Hys) in the analysis and search menus while the waveform acquisition is in progress and the trigger type is set to I<sup>2</sup>C, the waveform acquisition is restarted.
- Even if something other than I<sup>2</sup>C bus is selected in the analysis or search menu, the level and hysteresis settings of the analysis and search are set to the same value if the trigger level or hysteresis setting is changed.
- When the trigger level or hysteresis is changed by executing auto setup, the level and hysteresis settings of the analysis and hysteresis are also set to the same new value. This also applies when the setup information is initialized.
- Trigger hysteresis  $\frac{\cancel{A}}{\cancel{X}}$  and  $\frac{\cancel{X}}{\cancel{A}}$  correspond to 0.6 division and 1.0 division, respectively, of the analysis or search.

# 1.3 Analyzing the Data

You can set any of the channels, CH1 to CH4, to SDA or SCL and analyze the data. Because the I<sup>2</sup>C bus can be analyzed separately on Window 1 and Window 2, two waveforms can be analyzed.



## Procedure

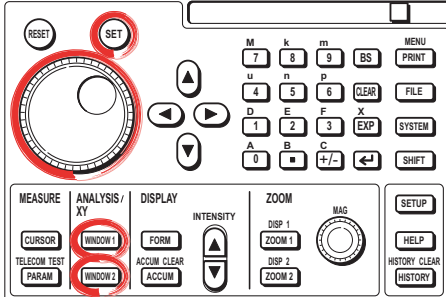

- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Analysis Conditions

1. Press **WINDOW1** or **WINDOW2**.
2. Press the **Type** soft key to display the Type menu.
3. Press the **Serial Bus** soft key.
4. Press the **Analyze** soft key to display the Analyze menu.
5. Press the **Mode** soft key to display the Mode menu.
6. Press the **I<sup>2</sup>C** soft key.

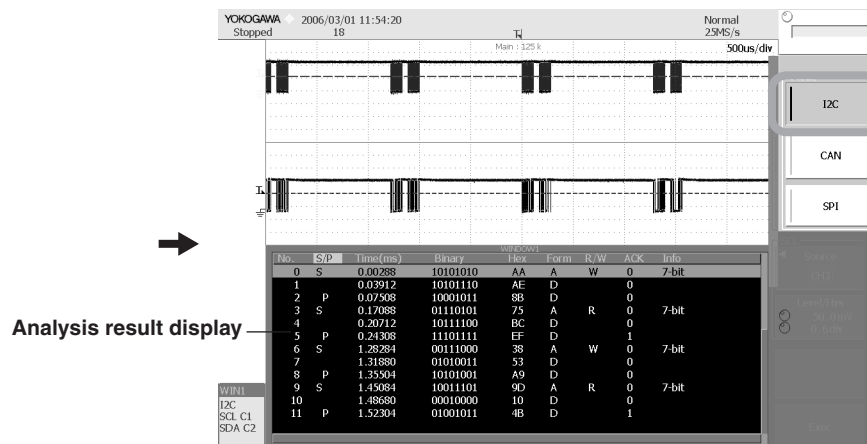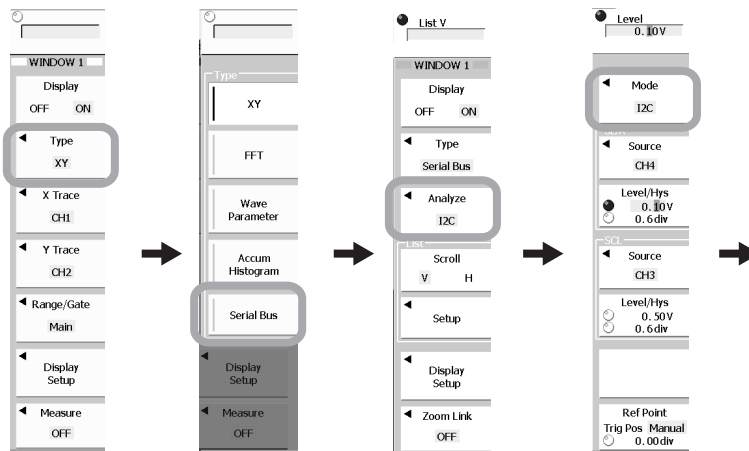

**Setting the Data Channel (SDA)**


7. Press the **Source** soft key under SDA to display a data channel menu.
8. Select the data channel from CH1 to CH4 and M1 to M4 (computation channels).

- **Setting the Level**

9. Press the **Level/Hys** soft key under SDA to activate the level.
10. Turn the **rotary knob** to set the threshold level.

- **Setting the Hysteresis**

11. Press the **Level/Hys** soft key under SDA to activate the hysteresis.
12. Turn the **rotary knob** to set the hysteresis.

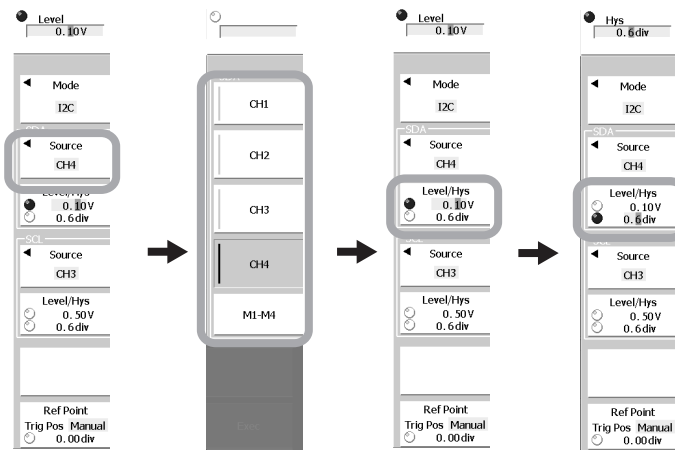**Setting the Clock Channel (SCL)**


13. Press the **Source** soft key under the SCL to display a clock channel menu.
14. Select the clock channel from CH1 to CH4 and M1 to M4 (computation channels).

- **Setting the Level**

15. Press the **Level/Hys** soft key under SCL to activate the level.
16. Turn the **rotary knob** to set the threshold level.


- **Setting the Hysteresis**

17. Press the **Level/Hys** soft key under SCL to activate the hysteresis.
18. Turn the **rotary knob** to set the hysteresis.

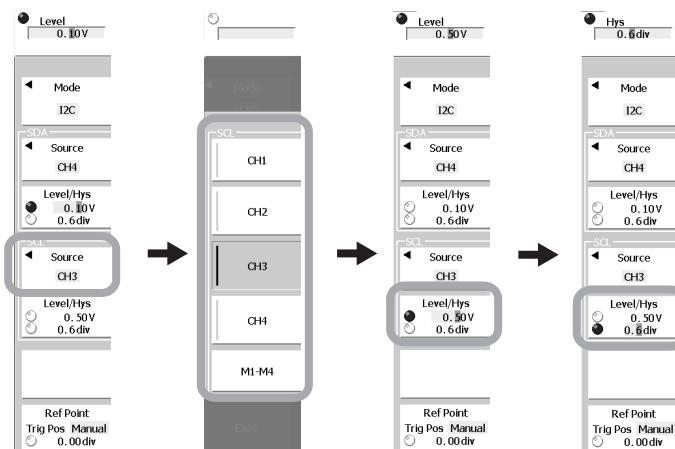


**Setting the Analysis Reference Point**

19. Pressing the **Ref Point** soft key to select Trig Pos or Manual.  
If you selected Manual, turn the rotary knob to set the reference point in the range of  $\pm 5.00$  divisions.



**Display the Analysis Results**

20. Press the **ESC**.
21. Press the **Scroll** soft key to select V (scroll vertically) or H (scroll horizontally).
22. Press the **Setup** soft key to display a menu used to set the analysis display.
23. Press the **Mode** soft key to select Simple (simple display) or Detail (detailed display).
24. Press any of the soft keys **1**, **10**, **100**, **1000**, and **10000** to set the step number for scrolling. The display scrolls according to the specified number.
25. Press **ESC**.
26. Press the **Display Setup** soft key to display the Display Setup menu.
27. Press the **VT** soft key to select ON or OFF. If ON is specified, the waveform is displayed on a normal voltage-time axis.
28. Press the **ESC**.

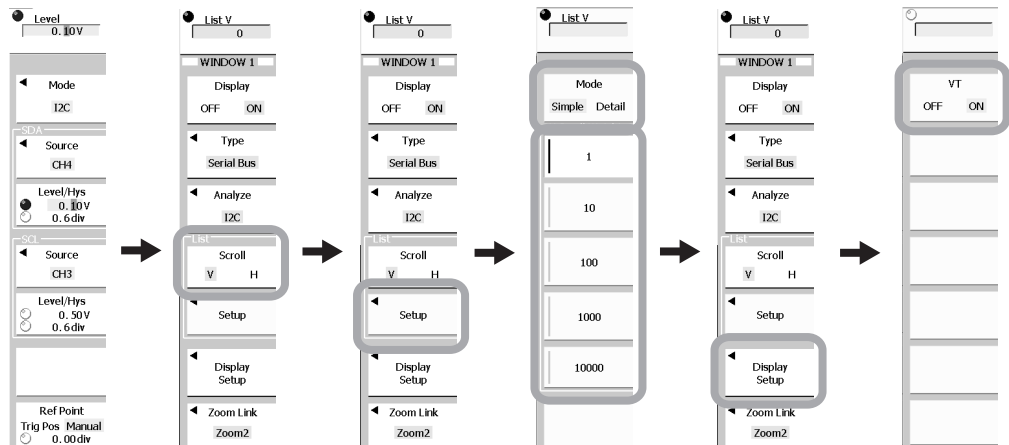


**Note**

The detailed analysis list can be saved directly to a storage medium in CSV format (.csv extension). For details, see section 1.5.

**Zoom Link**

29. Press the **Zoom Link** soft key to display the Zoom Link menu.
30. Press any of the soft keys, **OFF**, **Zoom1**, or **Zoom2** to set the link to the zoom screen. The zoom position (the center of the zoom box) can be moved to the head of the byte selected in the analysis result list by linking Zoom1 or Zoom2.

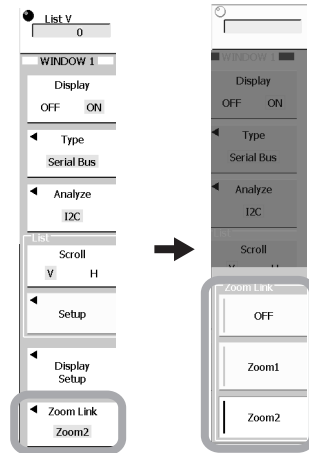**Explanation****Setting the Analysis Conditions**

You can set the following conditions.

**Data Channel (SDA)**

Select the data channel from CH1 to CH4 and M1 to M4. The clock channel and data channel can be set arbitrarily.

- **Level**

Set the level used to determine the data channel signal level (0 or 1).

Selectable range:  $\pm 10$  divisions around the vertical position

Resolution: 0.01 divisions (For example, the resolution for 2 mV/div is 0.02 mV.)

- **Hysteresis (Hys)**

Selectable range: 0.0 division to 4.0 divisions

Resolution: 0.1 divisions

**Clock Channel (SCL)**

Select the clock channel from CH1 to CH4 and M1 to M4. The clock channel and data channel can be set arbitrarily.

- **Level**

Set the level used to determine the rising or falling edge of the clock signal.

Selectable range:  $\pm 10$  divisions around the vertical position

Resolution: 0.01 divisions (For example, the resolution for 2 mV/div is 0.02 mV.)

- **Hysteresis (Hys)**

Selectable range: 0.0 division to 4.0 divisions

Resolution: 0.1 divisions


### 1.3 Analyzing the Data

#### Analysis Reference Point (Ref Point)

Select the analysis reference point from below.

Trig Pos	Sets the trigger position to the analysis reference point.
Manual	Manually set the analysis reference point. Selectable range: $\pm 5.00$ divisions, resolution: 0.01 divisions

Depending on the analysis reference point (Ref Point), the No. 0 byte in the analysis result list is as follows:



- (A): No. 0 byte -> Byte 1 (byte 2 is No. 1, byte 3 is No. 2, ...)
  - (B): No. 0 byte -> Byte 1 (byte 2 is No. 1, byte 3 is No. 2, ...)
  - (C): No. 0 byte -> Byte 2 (byte 1 is No. -1, byte 3 is No. 1, byte 4 is No. 2...)
  - (D): No. 0 byte -> Byte 5 (byte 1 is No. -4, ... byte 4 is No. -1, byte 6 is No. 1...)
- S: Start condition, P: Stop condition

#### Unification of the Trigger Setting of the I<sup>2</sup>C Bus Signal and the Setting of the I<sup>2</sup>C Bus Signal Analysis and Search

On products with software version 1.80 or higher, the trigger settings of the I<sup>2</sup>C bus signal on the menu that is entered through the ENHANCED key and the settings of the I<sup>2</sup>C bus signal analysis and search on the menu entered through the WINDOW1 and ZOOM1 key are common. For details, see page 1-13.

#### Analyzed Data

The following data can be analyzed:

- Waveform Data
  - Analysis can be performed regardless of whether the waveform acquisition is in progress. If the waveform acquisition is in progress, the analysis results are updated in real-time in sync with the displayed waveform. The waveform data stored in the history memory (waveform data of the record number selected using HISTORY menu > Select) is also analyzed.
- Loaded Acquisition Data (ACQ data)

#### Analysis Range

Up to 40000 bytes of analysis data can be displayed.

#### Analysis Data List (Analysis Result List)

The following information is displayed.

##### Simple Display

- Analysis number (No.): Up to 40000 points can be displayed.
- Start condition/Stop condition (S/P)
- Hexadecimal display of the data (Hex)
- Address/ Data (Form)
- Read/Write signal (R/W)
- Acknowledge bit condition (ACK)

Analysis number

Start condition

Hexadecimal display of data

Read/Write signal R: Read W: Write

No.	S/P	Hex	Form	R/W	ACK
9	I P	4B	D		1
10	S	F8	A	W	0
11		EB	D		0
12	P	21	D		0
13	S	9D	A	R	0
14		66	D		0
15	P	E2	D		1
16	S	38	A	W	0
17		9B	D		0
18	P	2C	D		0
19	S	6D	A	R	0
20		D7	D		0
21	P	4E	D		1

Stop condition


Acknowledge bit condition  
1: No acknowledge  
0: Acknowledge present

A: Address  
D: Data

**Detail Display**

- Analysis number (No.): Up to 40000 points can be displayed.
- Start condition/Stop condition (S/P)
- Time from the trigger position (Time(ms))
- Binary display of the data (Binary)
- Hexadecimal display of the data (Hex)
- Address/ Data (Form)
- Read/Write signal (R/W)
- Acknowledge bit condition (ACK)
- Data information (Info)

No.	S/P	Time(ms)	Binary	Hex	Form	R/W	ACK	Info
1	S	-2.46700	01110101	75	A	R	0	7-bit
2		-2.43100	10111100	BC	D		0	
3	P	-2.39500	11101111	EF	D		1	
4	S	-1.32301	00111000	38	A	W	0	7-bit
5		-1.28704	01010011	53	D		0	
6	P	-1.25104	10101001	A9	D		0	
7	S	-1.13904	10011101	9D	A	R	0	7-bit
8		-1.10304	00010000	10	D		0	
9	P	-1.06704	01001011	4B	D		1	
10	S	0.00496	11111000	F8	A	W	0	7-bit
11		0.04096	11101011	EB	D		0	
12	P	0.07696	00100001	21	D		0	
13	S	0.18896	10011101	9D	A	R	0	7-bit

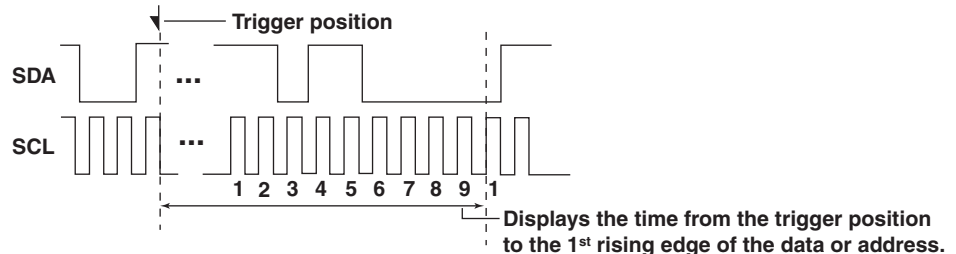**\* About the Time (ms) Display****Zoom Link**

Select from the following:

OFF Disables the zoom link function.

Zoom1 Links to Zoom1.


Zoom2 Links to Zoom2.

By default, WINDOW1 and WINDOW2 are linked to Zoom1 and Zoom2, respectively. If Zoom1 or Zoom2 is selected and you select (highlight) an arbitrary byte in the analysis result list, the zoom position (the center of the zoom box) of Zoom1 or Zoom2 moves to the head of that byte. Conversely, if you change the zoom position of Zoom1 or Zoom2, the highlight in the analysis result list moves to the byte that is shown in the zoom box of Zoom1 or Zoom2.

## 1.4 Searching the Waveform

You can search waveforms that match the specified conditions among the acquired waveforms. The setting of the search conditions are the same as the setting of the trigger conditions of section 1.2.

### Procedure

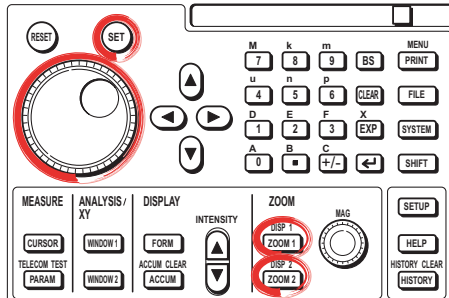


- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Search Conditions

1. Press **ZOOM1** or **ZOOM2** to display the ZOOM menu.
2. Press the **Setup** soft key to display the search condition menu.
3. Press the **Search Type** soft key.
4. Press the **Serial** soft key.
5. Press the **I<sup>2</sup>C** soft key.
6. Press the **Setup** soft key to display the search condition menu.

### Selecting the Search Mode

7. Press the **Mode** soft key to display the search mode selection menu.
8. Press the soft key corresponding to the desired search mode.

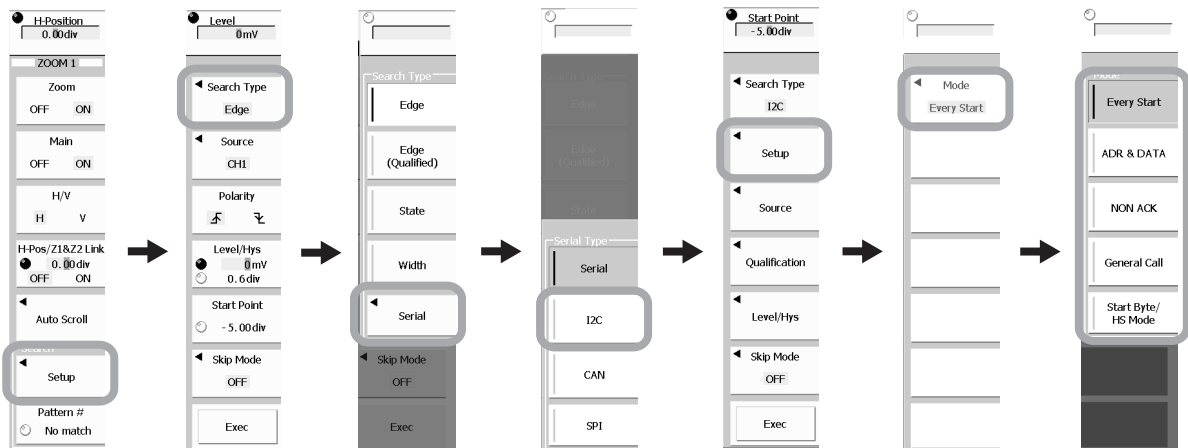

The procedure of setting the search conditions are the same as the procedure of setting the trigger conditions. See the pages indicated below according to the mode (the position of the soft keys may be different).

- Every Start (search the start condition): The setting procedure is complete.
- ADR & DATA (search an address pattern or data pattern): Page 1-3
- NON ACK (search the Nack): Page 1-5
- General Call (search the general call address): Page 1-5
- Start Byte/HS Mode (search the start byte or HS mode): Page 1-6



### Setting the Source Channel


9. Press the **Source** soft key to display the source channel menu.

### Setting the SDA Signal

10. Press the **SDA** soft key to display a menu used to select a channel to be the SDA signal and the level.
11. Press any of the soft keys **CH1** to **CH4** to assign the channel to the SDA signal.
12. Press the **Level** soft key. Turn the **rotary knob** to set the level used to determine high or low.

### Setting the SCL Signal

13. Press the **SCL** soft key to display a menu used to select a channel to be the SCL signal.
14. Like the SDA, set the channel to be the SCL signal and the level.

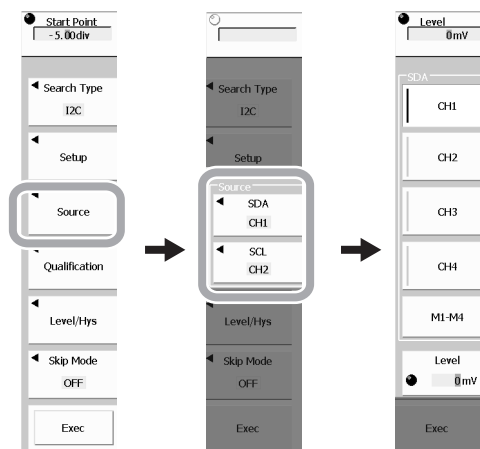


15. Press **ESC**.

### Setting the Qualification

You can search waveforms that meet the qualifications specified here and the search conditions specified in the Setup menu.

16. Press the **Qualification** soft key to display the Qualification menu.
17. Press a soft key of a channel that is not set to SDA or SCL, and set H, L, or X.
18. Press the **Logic** soft key to set whether to search the logic sum (OR) or logical product (AND) of the conditions specified in step 17.

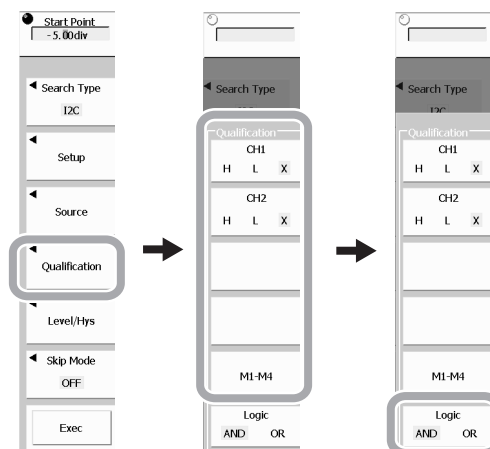

19. Press **ESC**.


## 1.4 Searching the Waveform

### Setting the Level and Hysteresis

20. Press the **Level/Hys** soft key.
21. Press the soft key corresponding to the channel you wish to configure.
22. Turn the **rotary knob** to set the level or hysteresis.  
If you change the level of the channel set to be the source channel, the level specified in the source channel settings (steps 12 and 14) is changed.
23. Press **ESC**.

### Setting the Skip Mode

24. Set the skip mode as necessary.  
Press the **Skip Mode** soft key to display the skip mode menu.
25. Press the **OFF**, **Hold Off**, or **Decimation** soft key.
26. Turn the **rotary knob** to set the time to skip or the search count.
27. Press **ESC**.

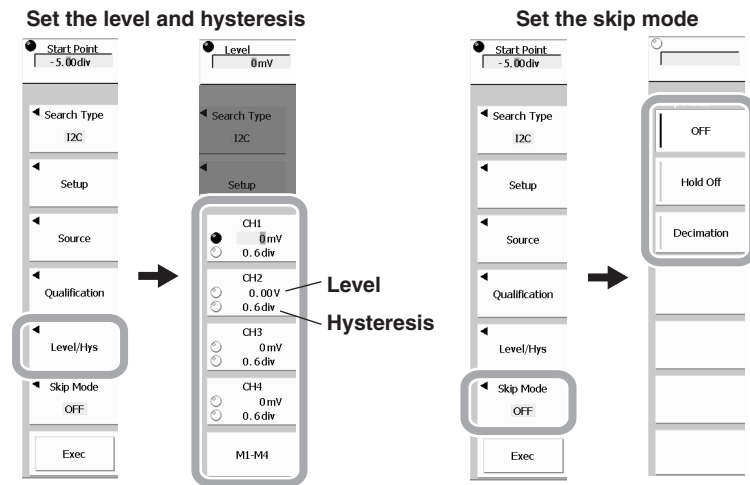

### Setting the Search Start Point


28. Turn the **rotary knob** to set the Start Point.

### Executing the Search

29. Press the **Exec** soft key. The section that meets the search conditions is shown on the ZOOM display.

### Viewing Search Points

30. Press **ESC**.
31. Press the **Pattern #** soft key.
32. Turn the **rotary knob** to select an arbitrary search point. The zoom position moves to the selected search point.

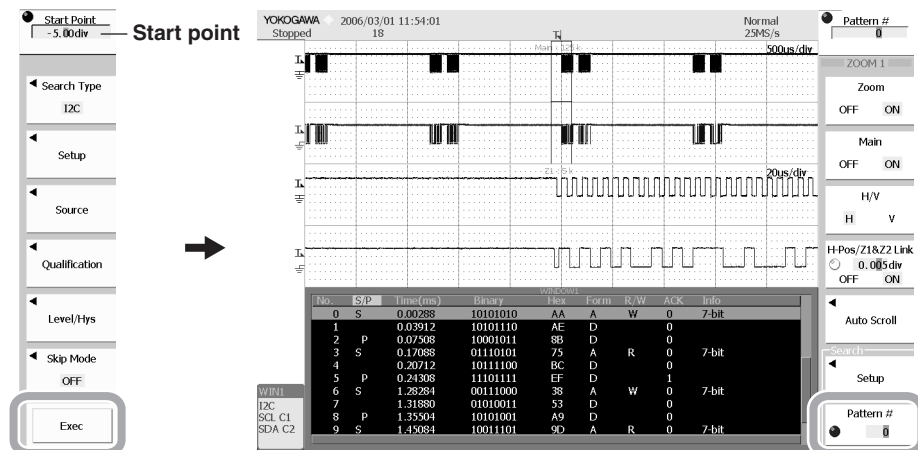

## Explanation

## Setting the Search Conditions

## Search Mode

You can select the search mode.

Every Start	Search on the start condition
ADR & DATA	Search an address pattern or data pattern
NON ACK	Search Nack
General Call	Search the general call address
Start Byte/HS Mode	Search the start byte or the master code of high speed mode

The search conditions are same as the trigger conditions. For details, see section 1.2.

## Source Channel, Qualification, Level, Hysteresis, Etc.

The settings for the source channel, qualification, level, hysteresis, and so on are the same as the settings of the analysis conditions. For details, see section 1.3.

## Skip Mode

After searching the position that meets the search conditions, the specified amount of time or the number of positions that match the search conditions are skipped.

OFF	Searches all sections that meet the search conditions.
Hold Off	Skips the search for the specified time.
Decimation	Skips the specified number of search positions.

## Search Start Point


Set the position to start the search in the range of  $\pm 5.00$  divisions.

## Search Point

When the search is executed, the zoom box (ZOOM1 or ZOOM2) moves to the data position where the conditions are met. The search point is the center of this zoom box. The search point varies depending on the selected search mode as follows:


## • Other than Every Start

As with the trigger point, the search point is the falling edge of the SDA signal.

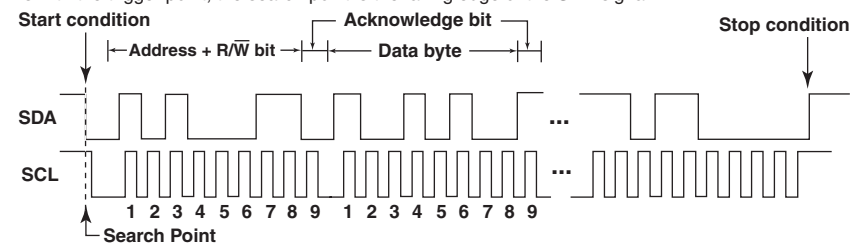

## • Mode: Every Start

The search point is the rising edge of the Acknowledge bit after the specified conditions are met. Below is an example when the Mode is set to ADR & DATA. It is similar in other search modes.

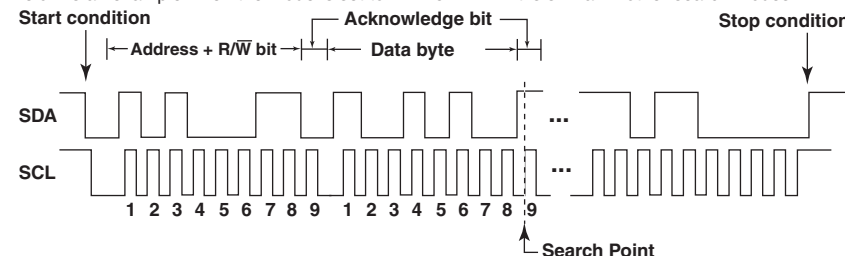

## Viewing Search Points

If you select an arbitrary search point using Pattern #, the zoom position moves to the selected search point. If the zoom link function is enabled (see page 1-19), the highlight in the analysis result list also moves to the byte containing the selected search point.

### **Unification of the Trigger Setting of the I<sup>2</sup>C Bus Signal and the Setting of the I<sup>2</sup>C Bus Signal Analysis and Search**


On products with software version 1.80 or higher, the trigger settings of the I<sup>2</sup>C bus signal on the menu that is entered through the ENHANCED key and the settings of the I<sup>2</sup>C bus signal analysis and search on the menu entered through the WINDOW1 and ZOOM1 key are common. For details, see page 1-13.

## 1.5 Saving the Data of the Analysis Result List

### CAUTION

Do not remove the medium (disk) or turn OFF the power when the access indicator is blinking. Doing so can damage the storage medium or destroy the data on the medium.

### Procedure

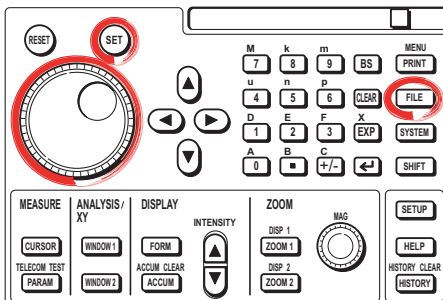

- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

- Press **FILE** to display the FILE menu.

### Setting the Storage Conditions


#### Selecting the Save Destination Medium and Directory

- Turn the **rotary knob** to select the save destination storage medium.
- Press the **Open** soft key to confirm the medium.

To store the data in a directory on the storage medium, select the directory in the same manner as step 2. Then, press the **Open** soft key to confirm the directory.

The selected medium/directory is displayed in "Path=....." located in the upper-left of the File List window.

Press the **UP** soft key to return to the next higher directory.

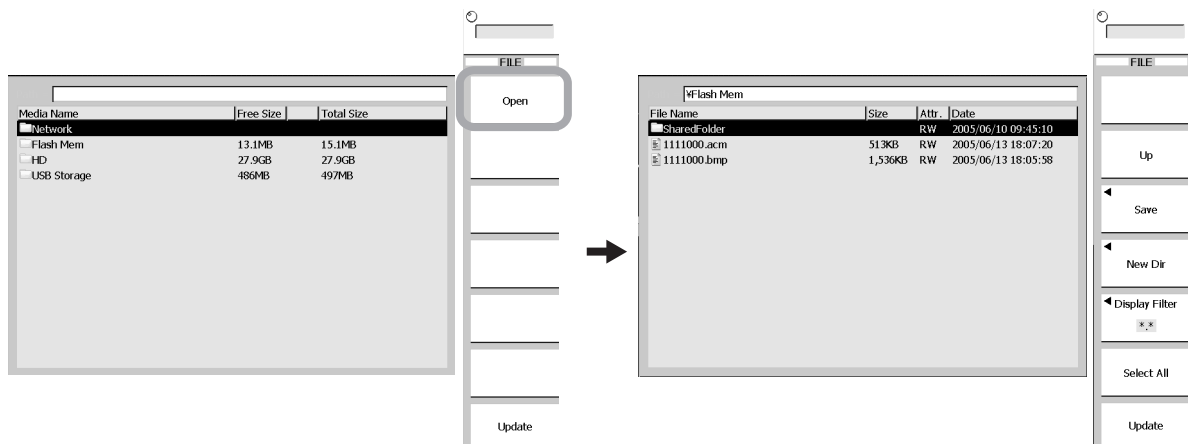


## 1.5 Saving the Data of the Analysis Result List

### Setting the Data Type

4. Press the **Save** soft key to display the file name menu.
5. Press the **Data Type** soft key to display the data type selection menu.
6. Press the **Next 1/2** soft key.
7. Press the **Serial Bus** soft key.


### Selecting the Window to Be Saved

8. Press the **Source** soft key to select Ana1 (WINDOW1) or Ana2 (WINDOW2) to be saved.

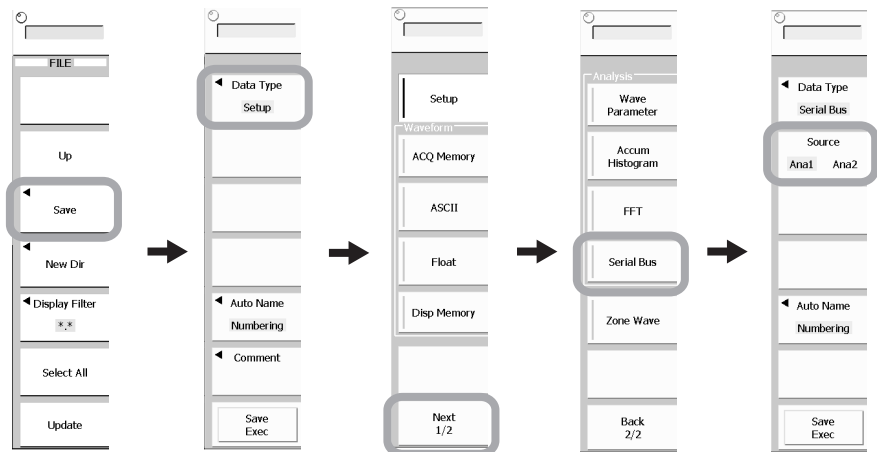

### Setting the File Name

9. Press the **Auto Name** soft key to display a menu used to select the method of setting the file name.
10. Press the **OFF**, **Numbering**, or **Date** soft key.
  - If you select Numbering, a sequence number is automatically appended to the specified file name. Proceed to step 11.
  - If you select Date, the date on which the data is saved is the file name. Proceed to step 12.
11. Press the **File Name** soft key.
12. Enter the file name according to the procedure given in section 4.2 in the *User's Manual (IM701310-01E)*.
13. Press the **Enter** to confirm the entered file name.

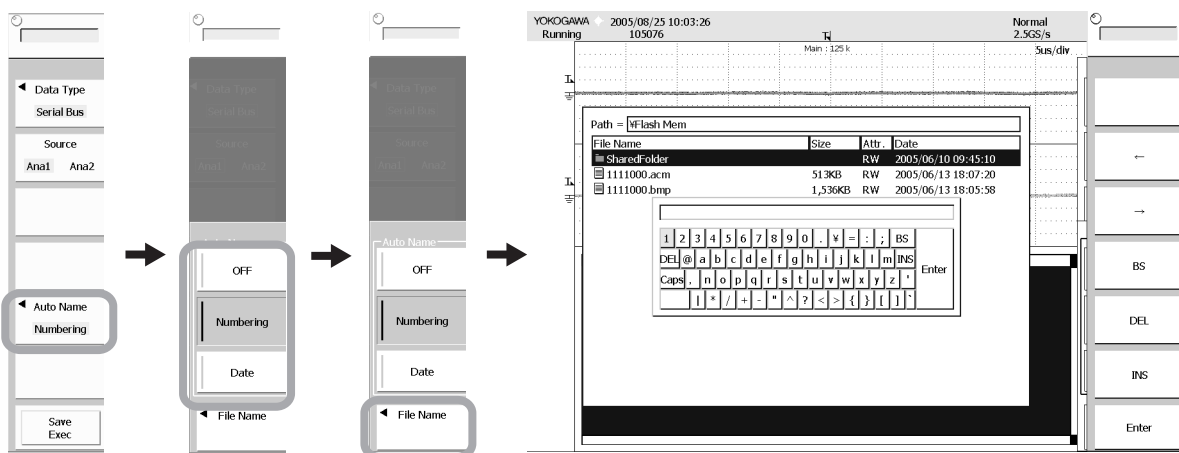

14. Press **ESC**.

### Executing the Save Operation

- Press the **Save EXEC** soft key. The data is saved to the directory indicated by Path=..... At the same time, the Save EXEC soft key changes to the Abort soft key. A media access icon appears at the upper left corner of the screen while the save operation is in progress.

When you abort the save operation, press the **Abort** soft key. The save operation is aborted. At the same time, the Abort soft key changes to the Save EXEC soft key.



### Explanation

The analysis results (the data of detailed display) can be saved in CSV format to a specified storage medium. The extension is .csv. Data in CSV format is a text file with data separated by commas. It is one of the common data formats used to convert data between spreadsheet and database applications.

### Setting the Storage Conditions

#### Data to Be Saved (Source)

Select Ana1 or Ana2.

Ana1: Analysis result through the WINDOW1 key

Ana2: Analysis result through the WINDOW2 key

#### Selecting the Storage Medium and Directory (File)

The available storage medium is displayed in the File List window.

- Display examples of storage media
  - [Storage Card]: PC card
  - [HD]: Internal hard disk (option)
  - [NetWork]: Network drive (option)
  - [Flash Mem]: Internal memory
  - [USB Storage]: USB storage device

## 1.5 Saving the Data of the Analysis Result List

---


### Setting the File Name

You can specify the file name using up to 64 characters. The characters that can be used are 0-9, A-Z, %, \_, (, and ).

#### • Auto Naming

Select from the following three types.

- OFF: The name specified by File Name is assigned.
- Numbering: Files are automatically named with three digit numbers from 000 to 999. You can specify a common name (up to 5 characters, specified through File Name) that is placed before the number.
- Date: Files are automatically named using eight characters (base 36 consisting of 0 to 9 and A to Z) based on the date and time. (The file name specified by File Name is void.)

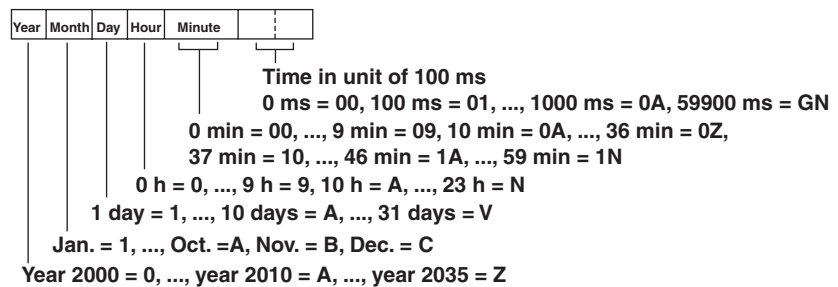

### Notes When Saving Data

The number of directories and files that can be displayed in the file list is 2500. If the number of directories and files in a directory exceeds 2500, the file list randomly displays 2500 of the directories and files.

#### Note

---

- An error occurs, if a key other than the Abort key is pressed while saving a file.
  - File names are not case-sensitive. Comments are case-sensitive. In addition, the following names cannot be used due to limitations of MS-DOS.  
AUX, CON, PRN, NUL, CLOCK, LPT1, LPT2, LPT3, LPT4, LPT5, LPT6, LPT7, LPT8, LPT9, COM1, COM2, COM3, COM4, COM5, COM6, COM7, COM8, and COM9.
  - Make sure that the full path name (absolute path name from the root directory) is within 260 characters. If 260 characters is exceeded, an error occurs when you execute a file operation (save, copy, rename, create directory, etc.).  
Full path name: If you are operating a directory, specify up to the directory name. If you are operating a file, specify up to the file name.
  - The length of the character string displayed in the entry box of the keyboard that is shown on the screen is 36. If you use the auto naming function of file names, the following conditions are added.
    - If you set auto naming to Numbering, eight-character file names are used consisting of the first five characters entered as the file name and a three-digit serial number.
    - If auto naming is set to Date (date/time), the characters entered as the file name are not used. The file name will only consists of the date information.
-



**Saved Data**

Up to 40000 analysis results.

**Data Size**

Data size\* = (Number of bytes + 4) × 65 [bytes]

\* The data size is a reference value. It is not strictly warranted. Use it as a guideline when saving the data.

**Data Format**

		Binary display of the analysis result		Hexadecimal display of the analysis result		Acknowledge bit condition		
						1: No acknowledge 0: Acknowledge present		
Analysis								
Model Nam DL9000								
Model Ver *.*								
No.	S/P	Time(ms)	Binary	Hex	Form	R/W	ACK	Info
0	S	-4.92896	11110010	Bin F2 Hex	A	W	0	10-bit
1		-4.92064	00001111	Bin 0F Hex	A		0	
2		-4.91264	10110000	Bin B0 Hex	D		0	
3	P	-4.90456	01101100	Bin 6C Hex	D		0	
4	S	-4.82896	11110010	Bin F2 Hex	A	W	0	10-bit
5		-4.82064	00001111	Bin 0F Hex	A		0	

**Time from the trigger position**  
**Start condition (S)/ stop condition (P)**  
**Analysis number**

**Address type**  
**Condition of the data direction bit (W: write, R: data request)**  
**Data format**  
**A: address, D: data**

## 1.6 Error Messages

A message may appear during operation. This section describes the meanings of the messages and their corrective actions. This section lists only the error messages related to the I<sup>2</sup>C Bus signal analysis function. There are other error messages related to the DL9000 and communications. These messages are described in the *User's Manual (IM701310-01E)* and the *Communication Interface User's Manual (IM701310-17E)*. You can set the messages to be displayed in English or Japanese. For the procedure of setting the message language, see section 17.1, "Changing the Message Language and Turning ON/OFF the Click Sound" in the *User's Manual (IM701310-01E)*. If the corrective action requires servicing, contact your nearest YOKOGAWA dealer for repairs.

Code	Messages	Corrective Action	Page
58	Search executed is completed, but no record was found that matched the pattern.	–	1-20
506	Save data do not exist. Check the content to be saved.	Display the analysis result, and then execute the save operation again.	1-14, 1-25

## 2.1 Overview of the CAN Bus Signal Analysis Function

### CAN Bus Signal Analysis Function

CAN stands for Controller Area Network. It is a serial communication protocol standardized internationally by the ISO (International Organization for Standardization). By using this function, data can be analyzed while displaying the signal waveforms on the CAN bus as analog waveforms. In addition, synchronized monitoring of the data on the CAN bus and the analog waveform is possible.


The CAN bus signal analysis function consists of the following four main functions.

#### Trigger Function <See page 2-5 for the operating procedure>

By setting the ID bit pattern, DLC, Data, and ACK slot status of the CAN bus, a trigger can be activated on a specific data frame or remote frame. Up to four ID/Data conditions can be specified allowing triggers to be activated on their OR conditions.

In addition, the SOF (Start of Frame) or error frame can be used as a trigger condition.

#### [Example] Standard Format of the Data Frame

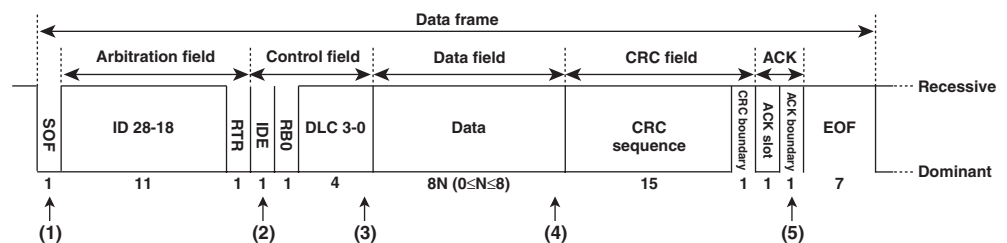

- (1) Trigger point when the trigger condition is set to SOF
- (2) Trigger point when the trigger condition is set only on the ID bit pattern
- (3) Trigger point when the trigger condition is set on the ID bit pattern and DLC
- (4) Trigger point when the trigger condition is set on the ID bit pattern and Data bit pattern
- (5) Trigger point when the trigger condition is set to the ACK slot state

A trigger can be activated on the combination of the trigger conditions of the CAN bus signal and analog signal (event interval trigger). For details on the event interval trigger, see section 6.14 in the *User's Manual (IM701310-01E)*.

#### Analysis Function <See pages 2-17 and 2-32 for the operating procedure>

This function analyzes the CAN bus signal data and shows a list of the analysis results. There are two types of analysis result lists: simple and detail. The simple list displays the analysis number, the type of analyzed frame, ID, Data, ACK slot status for each frame. The detail list displays the time from the trigger position, DLC, and CRC sequence in addition to the items displayed by the simple list. The data of the analysis result can be saved to an arbitrary storage medium in CSV format.

You can select an arbitrary frame in the analysis results list and automatically display the CAN bus signal for that frame (zoom link). The zoom position (the center of the zoom box) can be moved to the head of a specified field of the frame (field jump).

#### Search Function <See page 2-25 for the operating procedure>

A specific frame or field can be searched on the CAN bus signal data. When the search is executed, the zoom box moves to the data position where the conditions are met, and the data is displayed expanded in the zoom window (Zoom1 or Zoom2).


#### Stuff Bit Computation Function <See page 2-29 for the operating procedure>

Stuff bits within the CAN bus signals can be detected, and stuff bit waveforms can be displayed as math waveforms (stuff bit computation).

### High Speed CAN (ISO11898) and Low Speed CAN (ISO11519-2)

Two typical standards of the CAN physical layer are High speed CAN (ISO11898) and Low speed CAN (ISO11519-2).

In the figure below, the bus level is determined for both High and Low speed CAN according to the difference of potential between the CAN\_High and CAN\_Low busses.

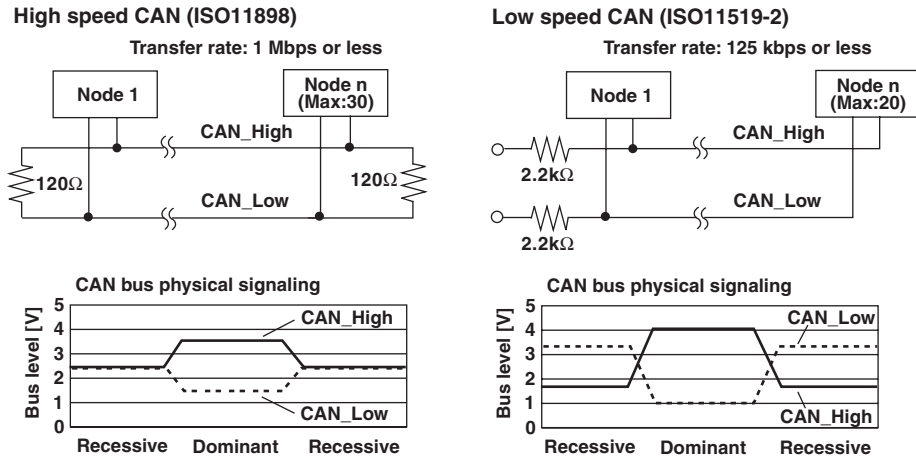

### Connecting the Probe

#### Probe to Be Used

A differential probe is used when measuring CAN bus signals.

Compatible differential probes: 701920 and 701922 by Yokogawa

#### Probe Connection Procedure

**When displaying the recessive voltage level higher than the dominant voltage level (Recessive: H)**

- **For a two wire system (differential)**  
Connect the differential probe negative (-) to CAN\_High, and the probe positive (+) to CAN\_Low.
- **For a one wire system (single-ended)**  
Connect the differential probe negative (-) to CAN\_High, and probe positive (+) to GND (ground potential).

**When displaying the recessive voltage level less than the dominant voltage level (Recessive: L)**


- **For a two wire system (differential)**  
Connect the differential probe negative (-) to CAN\_Low, and the probe positive (+) to CAN\_High.
- **For a one wire system (single-ended)\***  
Connect the differential probe negative (-) to GND (ground potential), and probe positive (+) to CAN\_High.

\* In this case, the passive probe (model 700988) can be connected to CAN\_High.

## 2.2 Setting the CAN Bus Signal Acquisition Conditions

With the CAN bus signal analysis function, you can acquire CAN bus signals using specific frames of the CAN bus as trigger conditions.

### Procedure



- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Trigger Conditions of the CAN Bus Signal


1. Press **ENHANCED**. The ENHANCED menu appears.
2. Press the **Type** soft key. The trigger type selection menu appears.
3. Press the **CAN** soft key.

### Selecting the Trigger Mode

4. Press the **Mode** soft key. A menu used to select the trigger mode of the CAN bus signal appears.
5. Press the **SOF**, **Error Frame**, **ID Std/Data**, **ID Ext/Data**, or **ID/Data OR** soft key to set the trigger mode.

### Setting the Bit Rate and Sample Point

6. Press the **Rate/Sample** soft key.
7. Press the **Bitrate** soft key. The bit rate selection menu appears.
8. Press the **1Mbps**, **500kbps**, **250kbps**, **125kbps**, **83.8kbps**, or **User** soft key to select the bit rate. If you select User, press the **Bitrate** soft key and turn the **rotary knob** to set an arbitrary value.
9. Press the **Sample Point** soft key.
10. Turn the **rotary knob** to set the sample point.

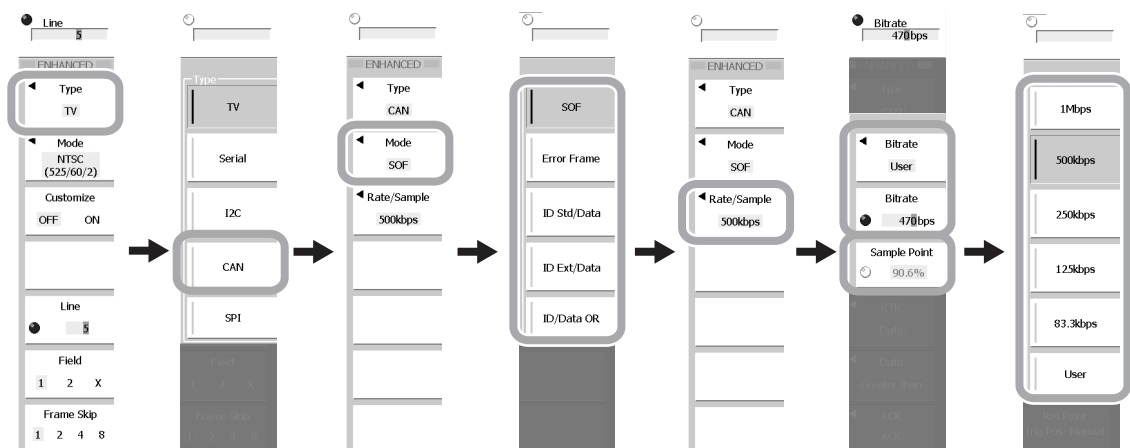

Proceed to the following pages depending on the trigger mode you selected in step 5.


- SOF (trigger on the Start of Frame): You are done with the settings.
- Error Frame (trigger on an error frame): You are done with the settings.
- ID Std/Data (trigger on the data/remote frame (ID: standard format)): Step 11
- ID Ext/Data (trigger on the data/remote frame (ID: extended format)): Step 11
- ID/Data OR (trigger on the OR condition of multiple data/remote frames): Step 30

## 2.2 Setting the CAN Bus Signal Acquisition Conditions

### • If You Selected ID Std/Data or ID Ext/Data in Step 5

#### Setting the ID Bit Pattern


11. Press the **Set ID** soft key. The ID setup screen appears.
12. Use the **rotary knob**, **arrow** keys, and **SET** key to set the ID pattern.  
You can use the soft keys to change the format to binary or hexadecimal, move between bits, or clear all the bits (X).
13. Press **ESC**.

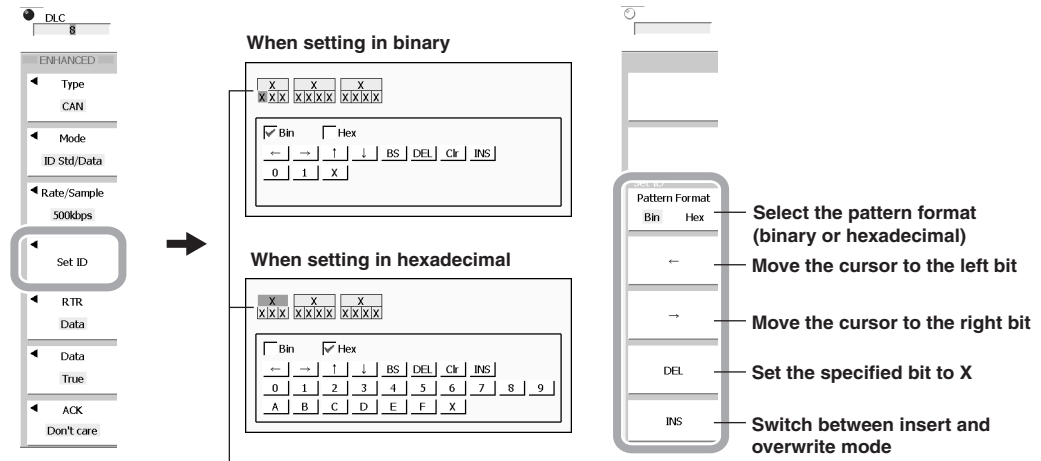

The figure above is the screen for ID Std/Data (ID: 11 bits).  
The ID is 29 bits for ID Ext/Data.

#### Setting the Remote Frame or Data Frame

14. Press the **RTR** soft key.
15. Press the **Don't care**, **Remote**, or **Data** soft key.
  - If you select Don't care, a trigger is activated on a remote frame or data frame. Proceed to step 28.
  - If you select Remote, a trigger is activated on a remote frame. Proceed to step 28.
  - If you select Data, a trigger is activated on a data frame. Proceed to step 16.

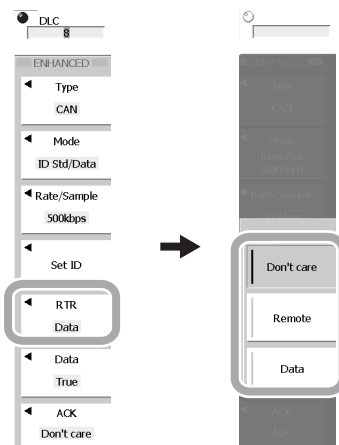

• **Setting the DLC**

16. Turn the **rotary knob** to set the DLC (number of valid bytes).

• **Setting the Data Field Condition**

17. Press the **Data** soft key.


18. Press the **Condition** soft key.

19. Press the **Don't care, True, False, Greater/Equal, Less/Equal, Between, or Out of Range** soft key.

- If you select Don't care, trigger is activated when the DLC matches. Proceed to step 28.
- If you select True, a trigger is activated when Data in the data field matches the specified bit pattern. Proceed to step 20.
- If you select False, a trigger is activated when Data in the data field does not match the specified bit pattern. Proceed to step 20.
- If you select Greater/Equal, a trigger is activated when Data in the data field is greater than or equal to the specified comparison data. Proceed to step 22.
- If you select Less/Equal, a trigger is activated when Data in the data field is less than or equal to the specified comparison data. Proceed to step 22.
- If you select Between, a trigger is activated when Data in the data field is greater than or equal to the specified comparison data Data1, and less than or equal to the comparison data Data2. Proceed to step 22.
- If you select Out of Range, a trigger is activated when Data in the data field is less than the specified comparison data Data1, or greater than the comparison data Data2. Proceed to step 22.

**Note**

For details on the trigger point for each condition, see page 2-15.

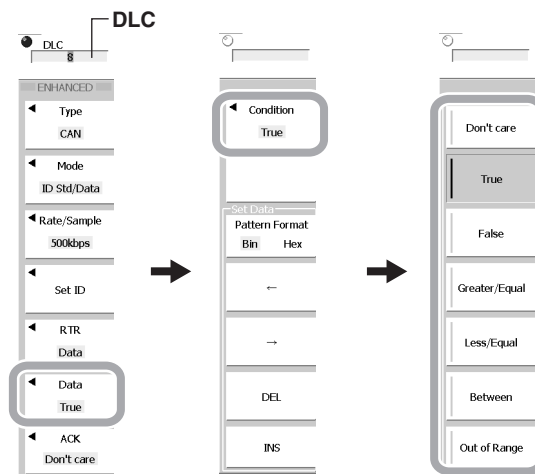


## 2.2 Setting the CAN Bus Signal Acquisition Conditions

- **Setting the Data Bit Pattern**



If you selected True or False in step 19, a screen used to set the Data bit pattern appears.

20. Use the **rotary knob**, **arrow** keys, and **SET** key to set the Data bit pattern. You can use the soft keys to change the format to binary or hexadecimal, move between bits, or clear all the bits (X).
21. Press **ESC**. Proceed to step 28.

### When setting in binary

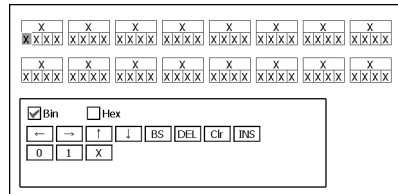

### When setting in hexadecimal

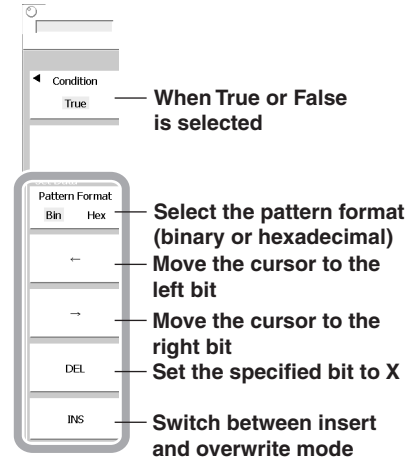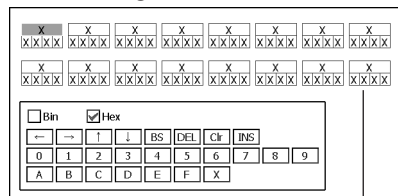

Set the pattern for the number of bytes specified by DLC.


- **Setting the Comparison Data**

If you select Greater/Equal, Less/Equal, Between, or Out of Range in step 19, a menu used to set the comparison data appears.

22. Press the **Byte Order** soft key to set the Endian of the value to Big or Little.
23. Press the **Sign** soft key to set the sign of the value to Sign (with a sign) or Unsign (without a sign).
24. Press the **MSB/LSB** soft key to set the MSB and LSB positions of the comparison data.
25. Press the **Data** soft key.
26. Turn the **rotary knob** to set the comparison data (Data, Data1, and Data2) in decimal notation.

If you select Greater/Equal or Less/Equal, set Data. If you select Between or Out of Range, set Data1 and Data2.

27. Press **ESC**. Proceed to step 28.

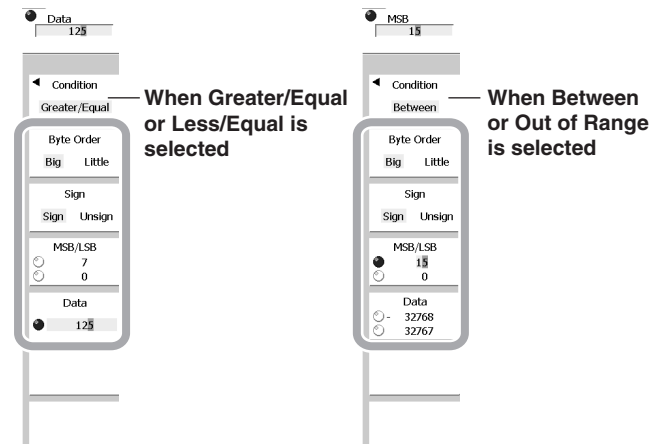




**Setting the ACK Slot**

28. Press the **ACK** soft key. The ACK slot setup menu appears.
29. Press the **Don't care**, **NON ACK**, **ACK**, or **NON ACK or ACK** soft key.
  - If you select Don't care, the bus level of the ACK slot is not used as a trigger condition.
  - If you select NON ACK, a trigger is activated when the bus level of the ACK slot is recessive.
  - If you select ACK, a trigger is activated when the bus level of the ACK slot is dominant.
  - If you select NON ACK or ACK, a trigger is activated when the ACK slot is recessive or dominant.

Proceed to step 33.

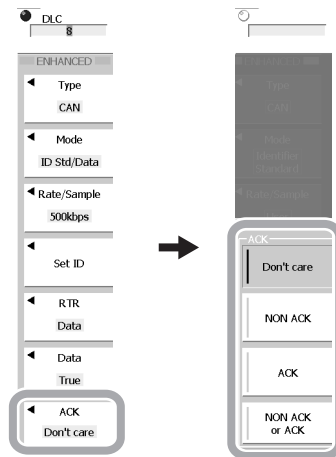

• **If You Selected ID/Data OR in Step 5**


**Setting the ID/Data for the OR Condition**

30. Press the **ID/Data 1**, **ID/Data 2**, **ID/Data 3**, or **ID/Data 4** soft key to select the ID/Data on which to set the OR condition.
31. Press the **ID/Data X** soft key (where X is a number between 1 and 4) to select ON (include in the OR condition) or OFF (not include in the OR condition).
32. Press the **Format** soft key to set the ID format to Std (standard format) or Ext (extended format).

The subsequent steps are the same as when you select ID Std/Data or ID Ext/Data in step 5. For the procedure, see steps 11 to 29 on page 2-4.

To activate a trigger on the OR condition of multiple ID/Data, repeat steps 30 to 32.

Proceed to step 33.

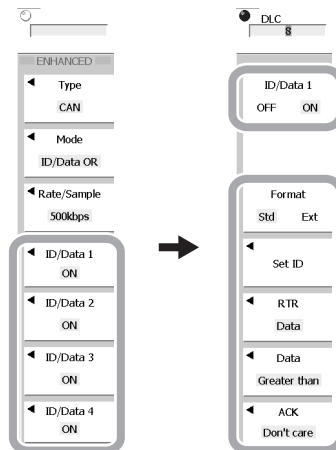

## 2.2 Setting the CAN Bus Signal Acquisition Conditions

---

### Setting the Source Channel


33. Press **SOURCE**. The SOURCE menu appears.

### Selecting the Source Channel

34. Press the **Source** soft key. A menu used to select the source channel of the CAN bus signal appears.
35. Press any of the soft keys **CH1** to **CH4** to select the source channel.

### Selecting the Bus Level

36. Press the **Recessive** soft key to select H (set the recessive electric potential higher than the dominant electric potential) or L (set the recessive electric potential less than the dominant electric potential).

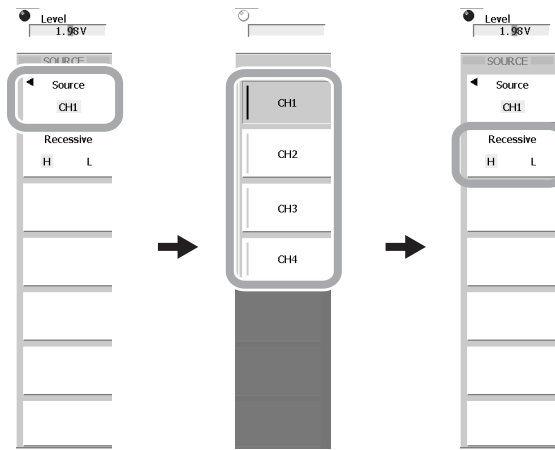

**Setting the Level, Coupling, HF Rejection, and Hysteresis**

37. Press **LEVEL/COUPLING**. The LEVEL/COUPLING menu appears.

**Selecting the Channel to Be Configured**

38. Press the **CH** soft key. A menu used to select the channel appears.

39. Press any of the soft keys **CH1** to **CH4**.

**Setting the Level**

40. Turn the **rotary knob** to set the level used to determine high or low of the channel set in step 39.

**Setting the Coupling**

41. Press the **Coupling** soft key to set the input coupling to DC.


**Setting the HF Rejection**

42. Press the **HF Rejection** soft key. A menu used to select the HF rejection appears.

43. Press the **OFF**, **20MHz**, or **15kHz** soft key.

**Setting the Hysteresis**

44. Press the **Hysteresis** soft key to select the hysteresis.

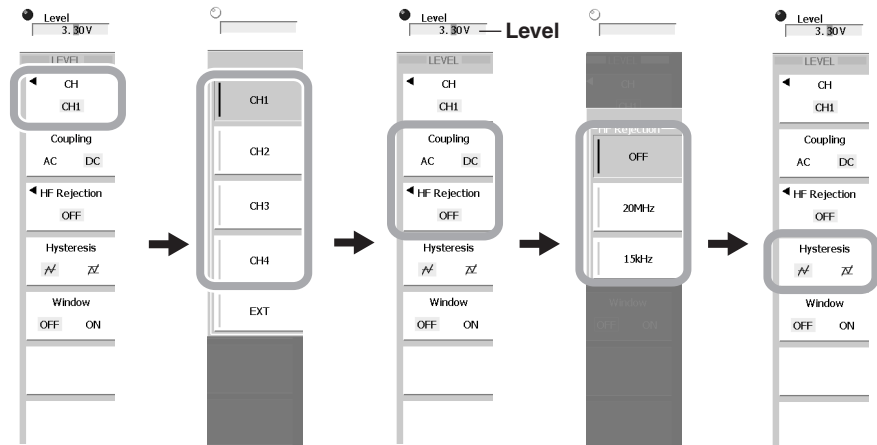

As necessary, repeat steps 38 to 44.

## 2.2 Setting the CAN Bus Signal Acquisition Conditions

### Explanation

#### Setting the Trigger Conditions of the CAN Bus Signal

##### Trigger Mode

The following trigger modes are available.

SOF	Activate a trigger on the Start of Frame (SOF).
Error Frame	Activate a trigger on an error frame.
ID Std/Data	Activate a trigger on a data frame or remote frame (ID: standard format) that matches the specified conditions.
ID Ext/Data	Activate a trigger on a data frame or remote frame (ID: extended format) that matches the specified conditions.
ID/Data OR	Activate a trigger on the OR condition of four types of data frames or remote frames. You can select standard or extended format for each ID.

For details on the trigger point for each trigger mode, see page 2-15.


##### Bitrate

Select the transfer rate of the CAN bus signal from 1Mbps, 500kbps, 250kbps, 125kbps, 83.8kbps, and User. If you select User, you can set an arbitrary value in the range of 10k to 1M [bps] (0.1 kbps resolution).

##### Sample Point

Set the point used to judge the bus level (recessive or dominant) in the range of 18.8 to 90.6 [%].

In the trigger circuits of the instrument's CAN bus signal analysis function, the input CAN bus signal is sampled once per the internal clock, and the point of change from recessive to dominant is detected. The detected point is taken as 0%, and the point one bit time (the reciprocal of the specified bit rate) thereafter is taken as 100%, allowing expression of the sample point as a percentage.

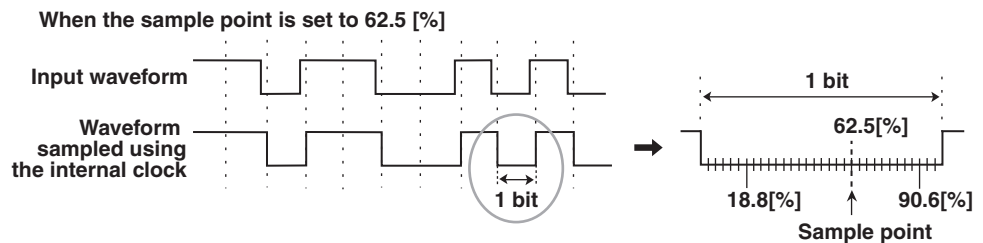

- **When the Trigger Mode Is Set to ID Std/Data or ID Ext/Data**

**ID Bit Pattern (Set ID)**

Set an 11-bit ID pattern if you select ID Std/Data or a 29-bit pattern if you select ID Ext/Data. Binary bit patterns are set using 0, 1, and X. Hexadecimal bit patterns are set using 0 to 9, A-F, and X. Matching of the specified ID bit pattern is a trigger condition.

**Note**

- If an ID bit pattern is set to X, the condition is assumed to be met regardless of the status of the corresponding bit.  
Binary: Condition met on either 0 or 1  
Hexadecimal: Condition met on any value (0 to 9 and A to F)
- If there is at least one "X" bit in a group of four bits of the ID bit pattern in the binary display, the corresponding hexadecimal display will show a "\$."

**Remote Frame or Data Frame (RTR)**

A trigger can be activated on the combination of remote frames or data frames and the ID bit pattern.

Don't care	Remote frames and data frames are used as trigger conditions.
Remote	Remote frames are used as trigger conditions.
Data	Data frames are used as trigger conditions.

The items below are set only when RTR is set to Data.

- **DLC**

Set the DLC (number of valid bytes) of the data field in the range of 0 to 8 bytes. The default value is 8 bytes.

- **Data Field Condition**

Select the data condition when using the data field as a trigger condition from the following:

Don't care	A trigger is activated when the DLC matches.
True	A trigger is activated when Data in the data field matches the specified bit pattern.
False	A trigger is activated when Data in the data field does not match the specified bit pattern.
Greater/Equal	A trigger is activated when Data in the data field is greater than or equal to the specified comparison data.
Less/Equal	A trigger is activated when Data in the data field is less than or equal to the specified comparison data.
Between	A trigger is activated when Data in the data field is greater than or equal to the specified comparison data Data1, and less than or equal to the comparison data Data2.
Out of Range	A trigger is activated when Data in the data field is less than the specified comparison data Data1, or greater than the comparison data Data2.

If Data1 is set equal to Data2 for Between, a trigger is activated when the data of the data field is equal to Data1 which is equal to Data2.

**Data Bit Pattern (Set Data)**

Set the bit pattern only when Condition is set to True or False.

Set the Data bit pattern. Binary bit patterns are set using 0, 1, and X. Hexadecimal bit patterns are set using 0 to 9, A-F, and X. The length of the bit pattern is the number of bytes set by DLC.

**Note**

- If an Data bit pattern is set to X, the condition is assumed to be met regardless of the status of the corresponding bit.  
Binary: Condition met on either 0 or 1  
Hexadecimal: Condition met on any value (0 to 9 and A to F)
- If there is at least one "X" bit in a group of four bits of the Data bit pattern in the binary display, the corresponding hexadecimal display will show a "\$."

## 2.2 Setting the CAN Bus Signal Acquisition Conditions

### Comparison Data

Set the items below if Condition is set to Greater/Equal, Less/Equal, Between, or Out of Range.

- **Data, Data1, and Data2**

Set the value (Data, Data1, and Data2) that is compared against the Data in the data field in decimal notation. Set Data for Greater/Equal or Less/Equal. Set Data1 and Data2 for Between or Out of Range.


For the selectable ranges of Data, Data1, and Data2, see “Sign” below.

- **Byte Order**


Set the byte read order of the Data, Data1, and Data2 to Big Endian or Little Endian.

For example, when a node transmits four-byte data (12345678: hexadecimal notation), the image of the frame on the bus is as shown in the following figure.

- **Big Endian**

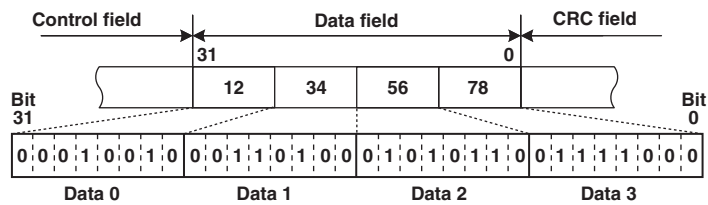

- **Little Endian**

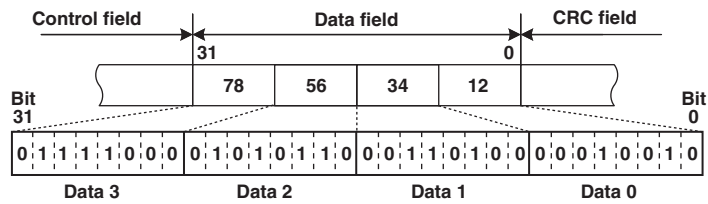

- **Sign**

Select whether to make Data, Data1, and Data2 signed numbers.

The selectable range of Data, Data1, and Data2 when you select Sign or Unsign is shown below.

Sign	-9E+18 to 9E+18
------	-----------------

Unsign	0 to 9E+18
--------	------------


The Data, Data1, and Data2 values are displayed using exponential notation when the values exceed seven digits (example: 1234567E+10).

• **MSB/LSB**


Set the bit positions of Data, Data1, and Data2 to be compared using MSB and LSB. The selectable range is 0 to 63 (the selectable range may be limited depending on the DLC setting).

For example, to compare only bits 5 to 20 of the four-byte data (12345678: hexadecimal notation), set LSB to 5 and MSB to 20. The bits of the data field that are compared for this case are as shown in the figure below for the different byte order settings (Big Endian and Little Endian).

• **Big Endian**




• **Little Endian**



**Note**

**Relationship between the DLC, MSB, LSB, Data, Data1, and Data2 values**

The relationship between the DLC, MSB, LSB, Data, Data1, and Data2 values is shown below.

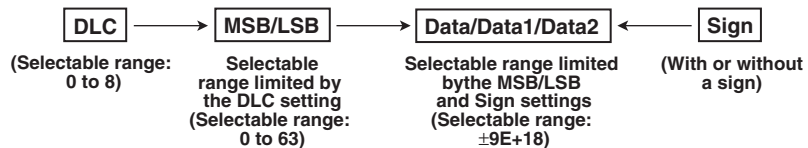

- [Example] When DLC is set to 2 bytes  
 $0 \leq \text{LSB} \leq \text{MSB} \leq 15$  (equivalent to 2 bytes)
- Sign (signed number):  $-32768 \leq \text{Data1} \leq \text{Data2} \leq 32767$
  - Unsign (unsigned number):  $0 \leq \text{Data1} \leq \text{Data2} \leq 65535$

**ACK Slot**

The bus level of the ACK slot (recessive or dominant) can be used as a trigger condition.

Don't care	The bus level of the ACK slot is not used as a trigger condition.
NON ACK	A trigger is activated when the bus level of the ACK slot is recessive.
ACK	A trigger is activated when the bus level of the ACK slot is dominant.
NON ACK or ACK	A trigger is activated when the bus level of the ACK slot is recessive or dominant.

## 2.2 Setting the CAN Bus Signal Acquisition Conditions

---

- **When the Trigger Mode Is Set to ID/Data OR**

**IDs Take the OR Logic (Edit Condition)**

Set four trigger conditions (ID/Data1 to ID/Data4) of data frames or remote frames. You can enable or disable each ID/Data condition. You can select standard or extended format for each ID.

**ID Format**

Set the ID format to Std (standard format) or Ext (extended format).

**ID Bit Pattern (Set ID)**

The details are the same as when the trigger mode is set to ID Std/Data or ID Ext/Data. For details, see page 2-11.

**Remote Frame or Data Frame (RTR)**

The details are the same as when the trigger mode is set to ID Std/Data or ID Ext/Data. For details, see page 2-11.

**ACK Slot**

The details are the same as when the trigger mode is set to ID Std/Data or ID Ext/Data. For details, see page 2-13.

**Source Channel**

The source channel of the CAN bus signal is set using the SOURCE menu that appears when you press the SOURCE key. The menu used to set the source channel of the CAN bus signal appears only when Type is set to CAN in the ENHANCED menu.

**Specifying the Source Channel**

The source channel is specified using the SOURCE menu.

**Bus Level (Recessive)**

Select the bus level from either of the following: In either case, the logical value is: recessive = 1 and dominant = 0.

H	The recessive electric potential is set higher than the dominant electric potential.
L	The recessive electric potential is set lower than the dominant electric potential.

**Trigger Level, Trigger Coupling, Etc.**

Set the trigger level, trigger coupling, HF rejection, and hysteresis of each channel. For details on these items, see the *User's Manual (IM701310-01E)*.



### Unification of the Trigger Setting of the CAN Bus Signal and the Setting of the CAN Bus Signal Analysis, Search and Stuff Bit Computation

The trigger settings of the CAN bus signal on the menu that is entered through the ENHANCED key and the settings of the CAN bus signal analysis, search, and stuff bit computation on the menu entered through the WINDOW1, ZOOM1, or M1 key are common. The CH1 to CH4 sources are the waveforms of which the settings are common.

#### Trigger settings of the CAN bus signal that are applied to the settings of analysis, search, and stuff bit computation

Level (trigger level), Hysteresis (trigger hysteresis), and Sample Point (The settings of the CAN bus signal analysis, search, and stuff bit computation are not applied to the trigger settings.)

#### Items for which the trigger settings, analysis settings, search settings, and stuff bit computation settings of the CAN bus signal are applied mutually

Source, Bitrate, and Recessive

#### Note


- The settings of the CAN bus signal analysis, search, and stuff bit computation on the menu entered through the WINDOW2, ZOOM2, and M2 to M4 keys are not made common. They are independent settings.
- If you change common items (excluding Level, Hys, and Sample Point) in the analysis, search, and stuff bit computation menus while the waveform acquisition is in progress and the trigger type is set to CAN, the waveform acquisition is restarted.
- Even if something other than CAN bus is selected in the analysis or search menu, the level and hysteresis settings of the analysis and search menus are set to the same value if the level or hysteresis setting is changed.
- If the trigger level or hysteresis is changed by executing auto setup, the level and hysteresis settings of the analysis and search are also set to the same new value. This also applies when the setup information is initialized.
- Trigger Hys  $\frac{\Delta}{\Delta}$  and  $\frac{\Delta}{\Delta}$  correspond to 0.6 division and 1.0 division, respectively, of the analysis, search, or stuff bit computation.

### Frame Format and Trigger Point


The following figure shows the format and trigger point of each frame.

#### Data Frame

##### • Standard format

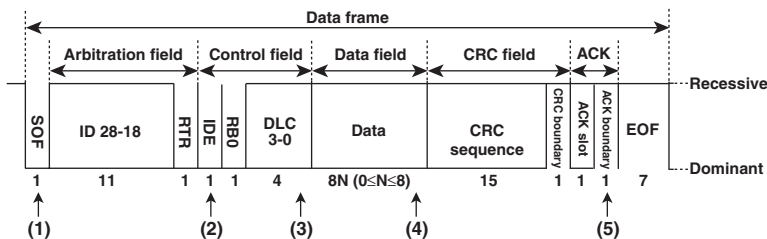

##### • Extended format

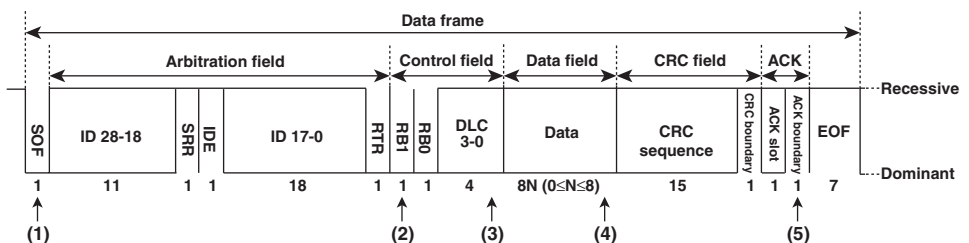

Items (1) to (5) above are the trigger points for the following conditions.


- (1) Mode: SOF
- (2) Mode: ID X\*, RTR: Don't care, and ACK: Don't care
- (3) Mode: ID X\*, RTR: Data, Condition: Don't care, and ACK: Don't care
- (4) Mode: ID X\*, RTR: Data, Condition: Other than Don't care, ACK: Don't care
- (5) ACK: Other than Don't care

\* ID X: For ID Std/Data, ID Ext/Data, or ID/Data OR


## 2.2 Setting the CAN Bus Signal Acquisition Conditions

### Remote Frame

#### • Standard format

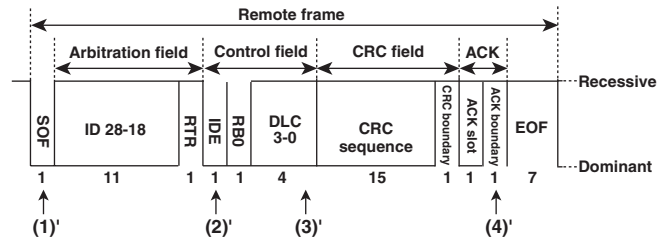

#### • Extended format

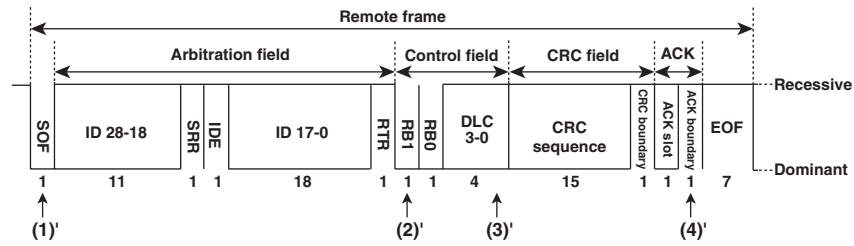


Items (1) to (5) above are the trigger points for the following conditions.

- (1)' Mode: SOF
- (2)' Mode: ID X\*, RTR: Don't care, ACK: Don't care
- (3)' Mode: ID X\*, RTR: Remote, ACK: Don't care
- (4)' ACK: Other than Don't care

\* ID X: For ID Std/Data, ID Ext/Data, or ID/Data OR

### Error Frame

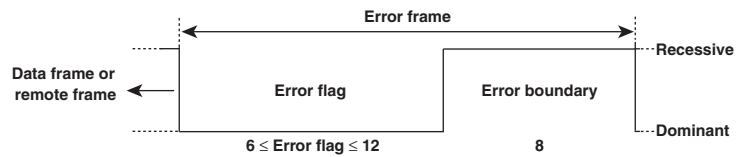


The trigger point is the 6<sup>th</sup> bit of the error flag when Mode is set to Error Frame.

## 2.3 Analyzing the Data

By setting analysis conditions, the CAN signal data stored to the acquisition memory can be analyzed.


### Procedure

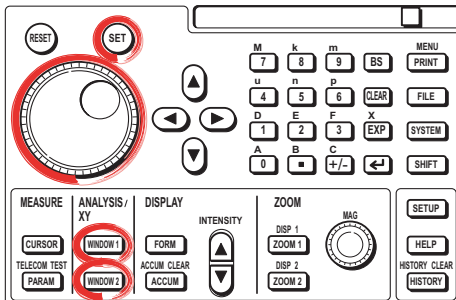

- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Analysis Conditions

1. Press **WINDOW1** or **WINDOW2**.
2. Press the **Type** soft key. The Type menu appears.
3. Press the **Serial Bus** soft key.
4. Press the **Analyze** soft key. The Analyze setup menu appears.
5. Press the **Mode** soft key. The Mode setup menu appears.
6. Press the **CAN** soft key.

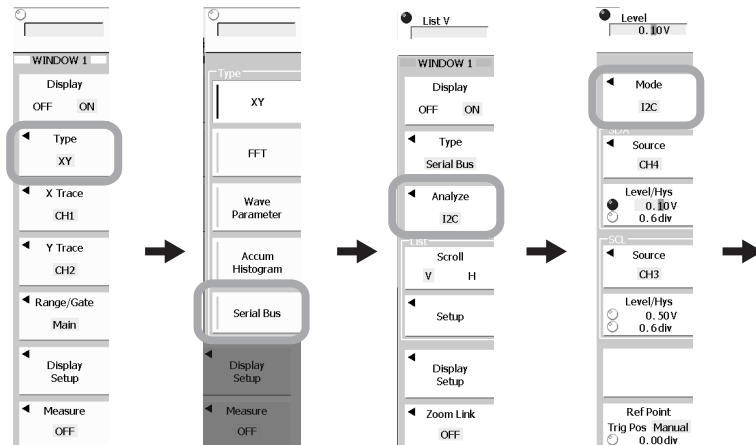

## 2.3 Analyzing the Data

### Setting the Bit Rate and Sample Point

7. Press the **Rate/Sample** soft key.
8. Press the **Bitrate** soft key. The bit rate selection menu appears.
9. Press the **1Mbps**, **500kbps**, **250kbps**, **125kbps**, **83.8kbps**, or **User** soft key to select the bit rate. If you select User, press the **Bitrate** soft key and turn the **rotary knob** to set an arbitrary value.
10. Press the **Sample Point** soft key.
11. Turn the **rotary knob** to set the sample point.
12. Press **ESC**.

### Setting the Source Channel

13. Press the **Source** soft key. The source channel setup menu appears.
14. Select the source channel from CH1 to CH4 and M1 to M4.

### Selecting the Bus Level

15. Press the **Recessive** soft key to select H (set the recessive electric potential higher than the dominant electric potential) or L (set the recessive electric potential less than the dominant electric potential).

### Setting the Level


16. Press the **Level/Hys** soft key to activate Level.
17. Turn the **rotary knob** to set the level.

### Setting the Hysteresis

18. Press the **Level/Hys** soft key to activate Hys (hysteresis).
19. Turn the **rotary knob** to set the hysteresis.

### Setting the Analysis Reference Point

20. Press the **Ref Point** soft key to select Trig Pos (set the analysis reference point to the trigger point) or Manual (set the analysis reference point manually).  
If you select Manual, turn the **rotary knob** to set the analysis reference point in the range of  $\pm 5.00$  divisions.

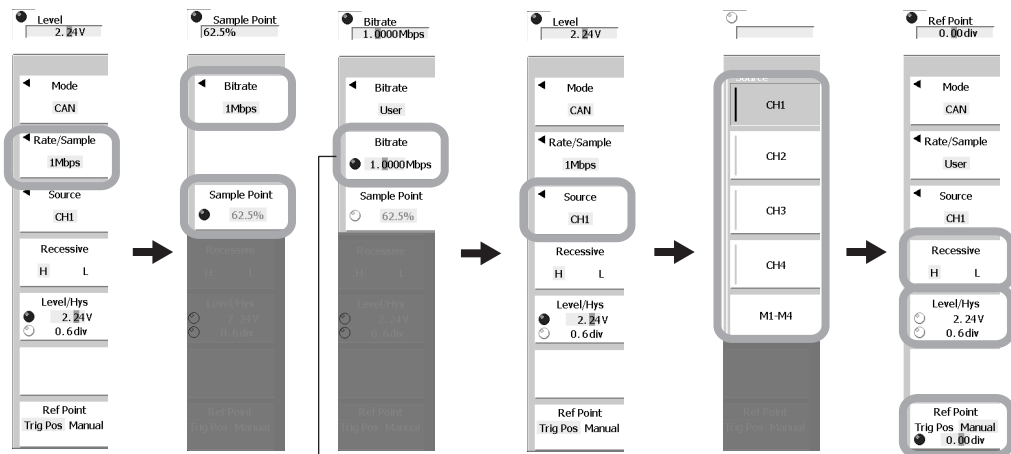


Displayed only when Bitrate is set to User.

### Display the Analysis Results

21. Press **ESC**.
22. Press the **Scroll** soft key to select V (scroll vertically) or H (scroll horizontally).
23. Press the **Setup** soft key. A menu used to set the analysis screen appears.
24. Press the **Mode** soft key to select Simple (simple display) or Detail (detailed display).
25. Press any of the soft keys **1**, **10**, **100**, **1000**, or **10000** to set the step number for scrolling. The display scrolls according to the specified number.
26. Press **ESC**.
27. Press the **Display Setup** soft key. The Display Setup menu appears.
28. Press the **VT** soft key to select ON or OFF. If ON is specified, the waveform is displayed on a normal voltage-time axis.
29. Press **ESC**.

### Note


The data of the simple display and detail display of the analysis results can be saved directly to a storage medium in CSV format (.csv extension). For details, see section 2.6.

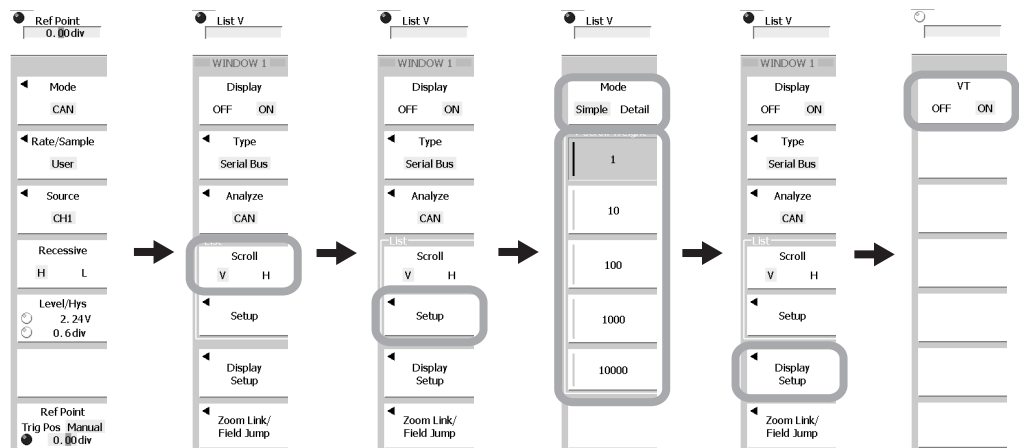

### Zoom Link and Field Jump

30. Press the **Zoom Link/Field Jump** soft key. The Zoom Link/Field Jump setup menu appears.
31. Press the **Zoom Link** soft key.
32. Press the **OFF**, **Zoom1**, or **Zoom2** soft key to set the link to the zoom window. If you select Zoom1 or Zoom2, proceed to step 33.
33. Press the **SOF**, **ID**, **Control Field**, **Data Field**, **CRC**, or **ACK** soft key under Field Jump.

If you select Zoom1 or Zoom2, set Scroll to V and turn the rotary knob to move the zoom position (the center of the zoom box) to the head of the frame highlighted in the analysis result list. If you press a soft key under Field Jump, the zoom position moves to the head of the corresponding field in the highlighted frame.

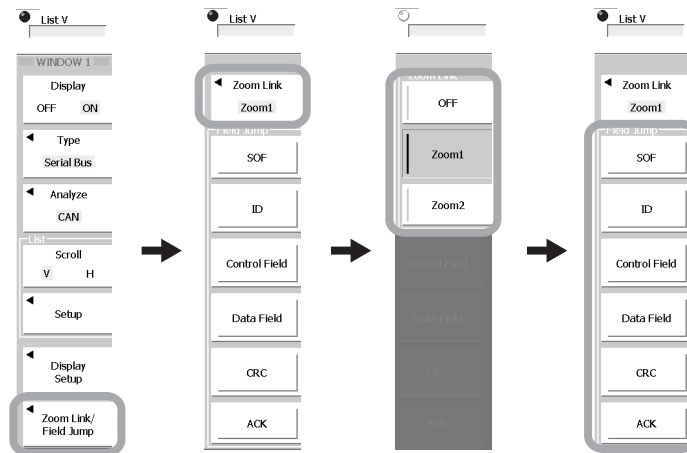

**Explanation****Setting the Analysis Conditions**

You can set the following conditions.

**Bitrate**

Select the transfer rate of the CAN bus signal from 1Mbps, 500kbps, 250kbps, 125kbps, 83.8kbps, and User. If you select User, you can set an arbitrary value in the range of 10k to 1M [bps] (0.1 kbps resolution).

**Sample Point**

The point at which the input CAN bus signal waveform changes from recessive to dominant is taken as 0%, and the point one bit time (the reciprocal of the specified bit rate) thereafter is taken as 100%, thereby allowing expression of the sample point as a percentage. The selectable range is 18.8 to 90.6 [%].

The details are the same as the trigger condition settings. See page 2-10.

**Source Channel**

Select the source channel from CH1 to CH4 and M1 to M4. The source channel can be set arbitrarily.

**Bus Level (Recessive)**

Select the bus level from either of the following: In either case, the logical value is: recessive = 1 and dominant = 0.

H	The recessive electric potential is set higher than the dominant electric potential.
L	The recessive electric potential is set lower than the dominant electric potential.

**Level**

Set the level used to determine the data channel signal level (0 or 1).

Selectable range:  $\pm 10$  divisions around the vertical position

Resolution: 0.01 divisions (For example, the resolution for 2 mV/div is 0.02 mV.)

**Hysteresis (Hys)**

Selectable range: 0.0 division to 4.0 divisions


Resolution: 0.1 divisions

**Analysis Reference Point (Ref Point)**

Select the analysis reference point from the following:

Trig Pos	Sets the trigger position to the analysis reference point.
Manual	Manually set the analysis reference point. Selectable range: $\pm 5.00$ divisions, resolution: 0.01 divisions

Depending on the analysis reference point (Ref Point), the No. 0 frame in the analysis result list is as follows:



(A): No. 0 frame -> Frame 2 (frame 1 is No. -1, frame 3 is No. 1, frame 4 is No. 2)

(B): No. 0 frame -> Frame 2 (frame 1 is No. -1, frame 3 is No. 1, frame 4 is No. 2)

(C): No. 0 frame -> Frame 3 (frame 1 is No. -2, frame 2 is No. -1, frame 4 is No. 1)

**Unification of the Trigger Setting of the CAN Bus Signal and the Setting of the CAN Bus Signal Analysis, Search and Stuff Bit Computation**

The trigger settings of the CAN bus signal on the menu that is entered through the ENHANCED key and the settings of the CAN bus signal analysis, search, and stuff bit computation on the menu entered through the WINDOW1, ZOOM1, or M1 key are common. For details, see page 2-15.

## 2.3 Analyzing the Data

### Analyzed Data

The following data can be analyzed:

- **Waveform Data**  
Analysis can be performed regardless of whether the waveform acquisition is in progress. If the waveform acquisition is in progress, the analysis results are updated in sync with the displayed waveform. The waveform data stored in the history memory (waveform data of the record number selected using HISTORY menu > Select) is also analyzed.
- **Loaded acquisition data (ACQ data).**

### Analyzed Frames

The following four types of frames are analyzed.

- **Data Frame**  
Detects the ID, Data, and CRC values and the presence of ACK.
- **Remote Frame**  
Detects the ID and CRC values and the presence of ACK.
- **Error Frame**  
Detects error flags.
- **Overload Frame**  
Detects overload flags.

### Analysis Range

Analysis is performed on up to 3000 frames before and after the trigger source frame.

### Analysis Data List (Analysis Result List)

The following information is listed.

#### Simple Display

- Analysis Number (No.)
- Frame type
- Hexadecimal display of ID
- Hexadecimal display of Data
- ACK slot state

Analysis number  
Frame type  
Hexadecimal display of ID  
Hexadecimal display of Data  
ACK slot state Y: ACK detected  
N: ACK not detected

No.	Frame	ID	Data	ACK
0	Data	100	01 A4	Y
1	Error		01	



**Detail Display**

- Analysis Number (No.)
- Frame type
- Time from the trigger position (Time (ms))
- Hexadecimal display of ID
- Hexadecimal display of DLC
- Binary display of Data (Bin)
- Hexadecimal display of Data
- Hexadecimal display of the CRC sequence
- ACK slot state

Analysis number  
Frame type  
Time from the trigger position to the head of the frame  
Hexadecimal display of ID  
Hexadecimal display of DLC  
ACK slot state

No.	Frame	Time(ms)	ID	DLC	Data(Bin)	Data	CRC	Ack
0	Data	-0.67973	100	3	11111111 00000001 10100100	FF 01 A4	6C6E	Y
1	Error	-0.03989			00000001	01		
2	Data	0.59994	00A	2	00000001 00000010	01 02	4A24	Y

Y: ACK detected  
N: ACK not detected

Hexadecimal display of the CRC sequence  
Hexadecimal display of Data  
Binary display of Data

- **Analysis Number (No.)**

Points before the analysis reference point (Ref Point) are counted as No. -1, No. -2, and so on. Points before the analysis reference points are counted as No. 0, No. 1, No. 2, and so on. Up to 3000 analysis results can be displayed in the range of -2999 to 2999.

Press the RESET key to highlight the No. 0 frame.

- **Frame Type**

The frames that can be analyzed are data frames, remote frames, error frames, and overload frames.

- **Time from the trigger position (Time (ms))**

Displays the time from the trigger position to the head of the frame in ms.

- **ID**

Displays the ID value (standard format (11 bits) or extended format (29 bits)) in hexadecimal notation.

- **DLC**

Displays the DLC (number of valid bytes) in hexadecimal notation.

- **Data**

Displays Data in hexadecimal or binary notation (only for Detail). The frame type is displayed only for data frames. Each byte is displayed on a line.

- **CRC Sequence**

Displays the CRC sequence in hexadecimal notation (only for Detail). The frame type is displayed only for data frames and remote frames.

- **ACK Slot State**

Displays "Y" when ACK is detected and "N" when ACK is not detected.

### Zoom Link and Field Jump

#### Zoom Link

Select from the following:

OFF	Disables the zoom link function.
Zoom1	Links to Zoom1.
Zoom2	Links to Zoom2.

By default, WINDOW1 and WINDOW2 are linked to Zoom1 and Zoom2, respectively. If Zoom1 or Zoom2 is selected and you select (highlight) an arbitrary frame in the analysis result list, the zoom position (the center of the zoom box) of Zoom1 or Zoom2 moves to the head of that frame. Conversely, if you change the zoom position of Zoom1 or Zoom2, the highlight in the analysis result list moves to the frame that is shown in the zoom box of Zoom1 or Zoom2.


#### Field Jump

When the zoom link function is enabled (Zoom Link set to Zoom1 or Zoom2), the zoom position can be moved to the head of the specified field of the frame that is highlighted in the analysis result list. Select the field from SOF, ID, Control Field, Data Field, CRC, or ACK.

## 2.4 Searching the Waveform

You can search waveforms that match the specified conditions among the acquired waveforms. The setup procedure of search conditions is the same as the setup procedure of trigger conditions explained in section 2.2.

### Procedure

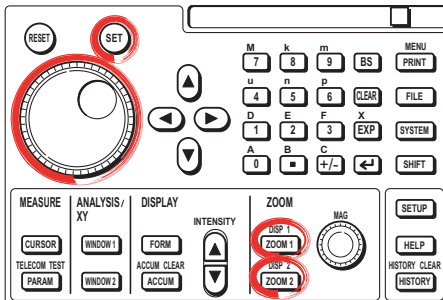


- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Search Conditions

1. Press **ZOOM1** or **ZOOM2**. The ZOOM menu appears.
2. Press the **Setup** soft key. The search condition setup menu appears.
3. Press the **Search Type** soft key.
4. Press the **Serial** soft key.
5. Press the **CAN** soft key.
6. Press the **Setup** soft key. The search condition setup menu appears.

### Selecting Search Mode


7. Press the **Mode** soft key. The search mode selection menu appears.
8. Press the soft key corresponding to the desired search mode.

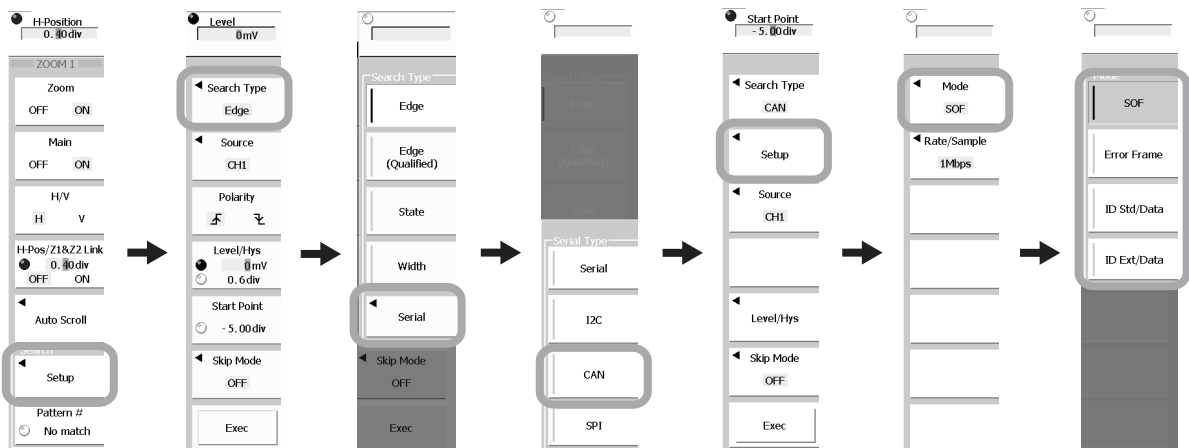

## 2.4 Searching the Waveform

### Setting the Bit Rate and Sample Point

9. Press the **Rate/Sample** soft key.
10. Press the **Bitrate** soft key. The bit rate selection menu appears.
11. Press the **1Mbps**, **500kbps**, **250kbps**, **125kbps**, **83.8kbps**, or **User** soft key to select the bit rate. If you select User, press the **Bitrate** soft key and turn the **rotary knob** to set an arbitrary value.
12. Press the **Sample Point** soft key.
13. Turn the **rotary knob** to set the sample point.

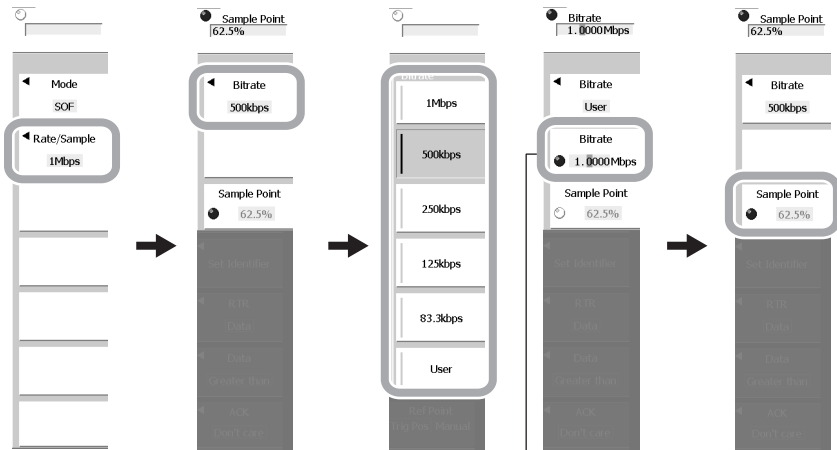

Displayed only when User is selected.

The setup procedure of other search conditions is the same as the setup procedure of trigger conditions. See the pages listed below depending on search mode. (The soft key positions may differ.)

- SOF (search the Start of Frame): You are done with the settings.
- Error Frame (search an error frame): You are done with the settings.
- ID Std/Data (search the data/remote frame (ID: standard format)): Page 2-4
- ID Ext/Data (search the data/remote frame (ID: extended format)): Page 2-4


### Setting the Source Channel

#### Selecting the Source Channel

14. Press **ESC** twice.
15. Press the **Source** soft key. The source channel setup menu appears.
16. Press any of the soft keys **CH1** to **CH4** or **M1** to **M4** to select the source channel.

#### Selecting the Bus Level

17. Press the **Recessive** soft key to select H (set the recessive electric potential higher than the dominant electric potential) or L (set the recessive electric potential less than the dominant electric potential).
18. Press **ESC**.

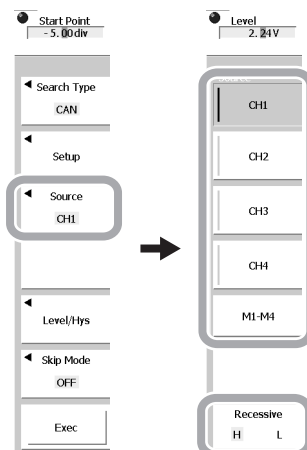


**Setting the Level and Hysteresis**

19. Press the **Level/Hys** soft key.
20. Press the soft key corresponding to the channel you wish to configure.
21. Turn the **rotary knob** to set the level or hysteresis.
22. Press **ESC**.

**Setting the Skip Mode**

23. Set the skip mode as necessary.  
Press the **Skip Mode** soft key. The skip mode setup menu appears.
24. Press the **OFF**, **Hold Off**, or **Decimation** soft key.
25. Turn the **rotary knob** to set the time to skip or the search count.
26. Press **ESC**.

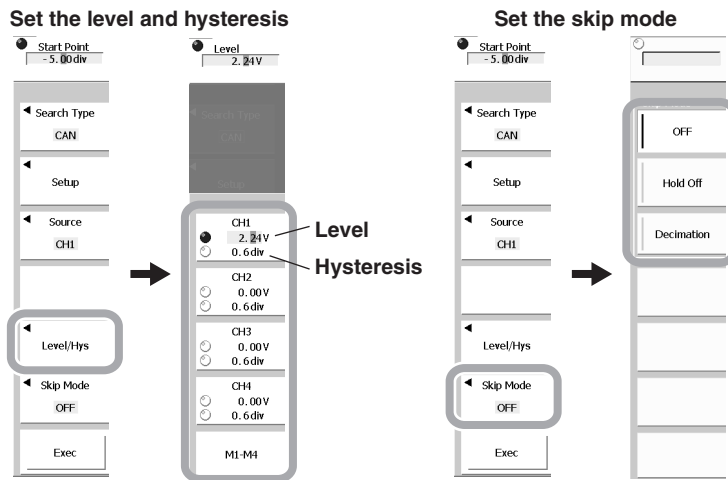

**Setting the Search Start Point**


27. Turn the **rotary knob** to set the search start point.

**Executing the Search**

28. Press the **Exec** soft key. The section that meets the search conditions is displayed expanded in the zoom window.

**Viewing Search Points**

29. Press **ESC**.
30. Press the **Pattern #** soft key.
31. Turn the **rotary knob** to select an arbitrary search point. The zoom position moves to the selected search point.

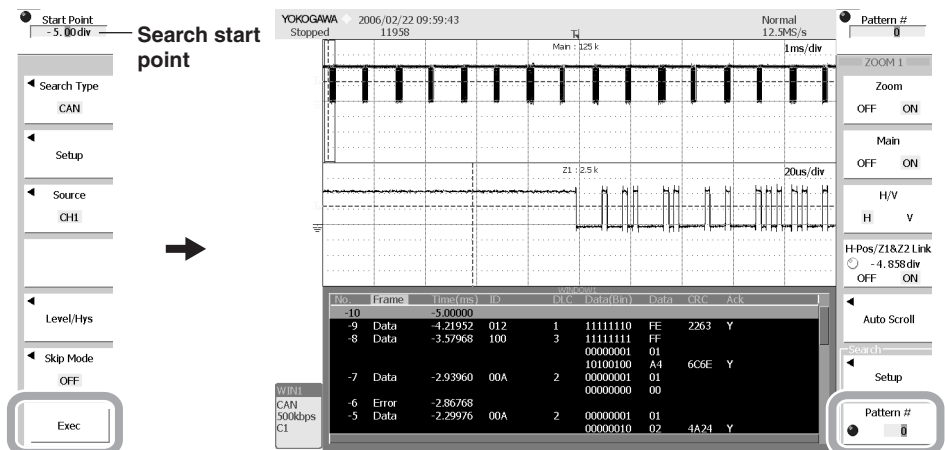

### Explanation

#### Setting Search Conditions

##### Search Mode

You can select the search mode from below.

SOF	Search the SOF (Start of Frame)
Error Frame	Search an error frame
ID Std/Data	Search a data frame or remote frame (ID: standard format) that matches the specified conditions.
ID Ext/Data	Search a data frame or remote frame (ID: extended format) that matches the specified conditions.

The settings of other search conditions are the same as the settings of trigger conditions. For details, see section 2.2.

##### Source Channel, Level, Hysteresis, Etc.

The settings for the source channel, level, hysteresis, and so on are the same as the settings of the analysis conditions. For details, see section 2.3.

##### Skip Mode

After searching the position that meets the search conditions, the specified amount of time or the number of positions that match the search conditions are skipped.

Select the skip mode from the following:

OFF	Searches all sections that meet the search conditions.
Hold Off	Skips the search for the specified time.
Decimation	Skips the specified number of search positions.

##### Search Start Point

Set the position to start the search in the range of  $\pm 5.00$  divisions.

##### Search Point

When the search is executed, the zoom box moves to the data position where the conditions are met. The search point is the center of this zoom box. The search point is set to the same position as the trigger position (see page 2-15).

##### Viewing Search Points

If you select an arbitrary search point using Pattern #, the zoom position moves to the selected search point. If the zoom link function is enabled (see page 2-24), the highlight in the analysis result list also moves to the frame containing the selected search point.


##### Unification of the Trigger Setting of the CAN Bus Signal and the Setting of the CAN Bus Signal Analysis, Search and Stuff Bit Computation

The trigger settings of the CAN bus signal on the menu that is entered through the ENHANCED key and the settings of the CAN bus signal analysis, search, and stuff bit computation on the menu entered through the WINDOW1, ZOOM1, or M1 key are common. For details, see page 2-15.

## 2.5 Performing Stuff Bit Computation

Stuff bits can be extracted from the CAN bus signal waveform and displayed as computed waveforms (MATH1 to MATH4).

### Procedure

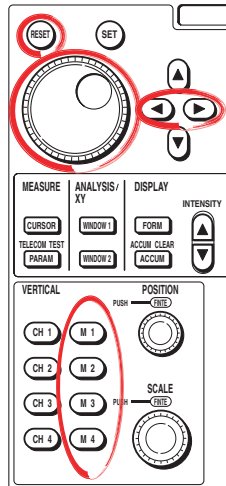

- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Stuff Bit Computation


1. Press any of the keys **M1** to **M4** to select the channel on which to display the stuff bit waveform.
2. Press the **Select** soft key to select MATH.

### Selecting the Operator

3. Press the **Operation** soft key. The operator selection menu appears.
4. Press the **Stuff Bit** soft key.
5. Press the **Setup** soft key. The stuff bit computation setup menu appears.

### Selecting the Waveform to Be Computed

6. Press the **Source** soft key. The search condition setup menu appears.
7. Press any of the soft keys **CH1** to **CH4** and **REF1-REF4** to waveform to be computed.

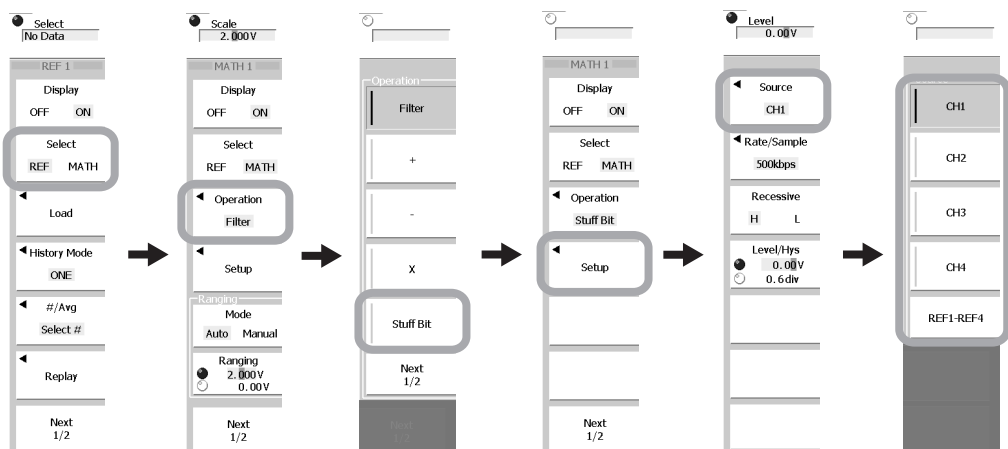

## 2.5 Performing Stuff Bit Computation

### Setting the Bit Rate and Sample Point

8. Press the **Rate/Sample** soft key.
9. Press the **Bitrate** soft key. The bit rate selection menu appears.
10. Press the **1Mbps**, **500kbps**, **250kbps**, **125kbps**, **83.8kbps**, or **User** soft key to select the bit rate. If you select User, press the **Bitrate** soft key and turn the **rotary knob** to set an arbitrary value.
11. Press the **Sample Point** soft key.
12. Turn the **rotary knob** to set the sample point.
13. Press **ESC**.

### Selecting the Bus Level


14. Press the **Recessive** soft key to select H (set the recessive electric potential higher than the dominant electric potential) or L (set the recessive electric potential less than the dominant electric potential).

### Setting the Level

15. Press the **Level/Hys** soft key to activate Level.
16. Turn the **rotary knob** to set the level.

### Setting the Hysteresis

17. Press the **Level/Hys** soft key to activate Hys (hysteresis).
18. Turn the **rotary knob** to set the hysteresis.

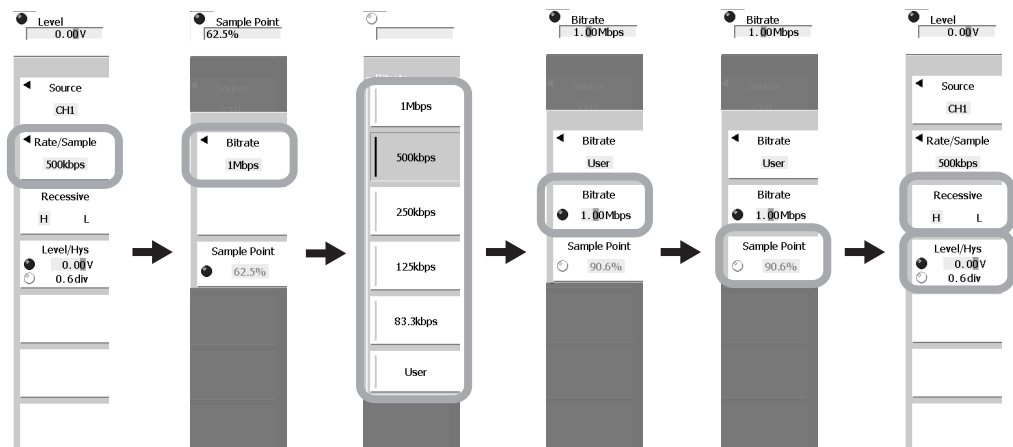


## Explanation

### Stuff Bit

In CAN communication, if five or more continuous bits between the Start of Frame and CRC sequence are at the same level, CAN inserts a bit (stuff bit) having the opposite logical value of the five previous bits for the next bit (6<sup>th</sup> bit).

The DL9040/DL9140/DL9240/DL9040L/DL9140L/DL9240L lets you extract stuff bits from the CAN bus signal waveform and display them as a MATH waveform.

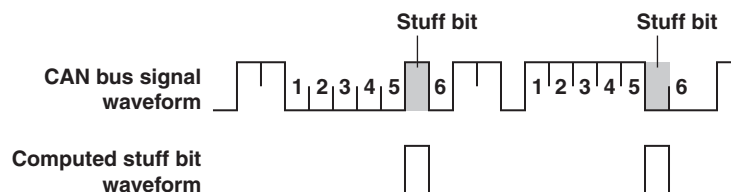



## Setting the Stuff Bit Computation

You can set the following conditions.

### Waveform to Be Computed (Source)

Select the source waveform for the stuff bit computation from CH1 to CH4 and REF1 to REF4. The default settings are MATH1: CH1, MATH2: CH2, MATH3: CH3, and MATH4: CH4.

### Bitrate

Select the transfer rate of the CAN bus signal from 1Mbps, 500kbps, 250kbps, 125kbps, 83.8kbps, and User. If you select User, you can set an arbitrary value in the range of 10k to 1M [bps] (0.1 kbps resolution).

### Sample Point

The point at which the input CAN bus signal waveform changes from recessive to dominant is taken as 0%, and the point one bit time (the reciprocal of the specified bit rate) thereafter is taken as 100%, thereby allowing expression of the sample point as a percentage. The selectable range is 18.8 to 90.6 [%].

The details are the same as the trigger condition settings. See page 2-10.

### Bus Level (Recessive)

Select the bus level from either of the following: In either case, the logical value is: recessive = 1 and dominant = 0.

H	The recessive electric potential is set higher than the dominant electric potential.
L	The recessive electric potential is set lower than the dominant electric potential.

### Level

Set the level used to determine the data channel signal level (0 or 1).

Selectable range:  $\pm 10$  divisions around the vertical position

Resolution: 0.01 divisions (For example, the resolution for 2 mV/div is 0.02 mV.)

### Hysteresis (Hys)

Selectable range: 0.0 division to 4.0 divisions

Resolution: 0.1 divisions

## Unification of the Trigger Setting of the CAN Bus Signal and the Setting of the CAN Bus Signal Analysis, Search and Stuff Bit Computation

The trigger settings of the CAN bus signal on the menu that is entered through the ENHANCED key and the settings of the CAN bus signal analysis, search, and stuff bit computation on the menu entered through the WINDOW1, ZOOM1, or M1 key are common. For details, see page 2-15.

## 2.6 Saving the Data of the Analysis Result List

### CAUTION

Do not remove the medium (disk) or turn OFF the power when the access indicator is blinking. Doing so can damage the storage medium or destroy the data on the medium.

#### Procedure

The procedure to save the data of the analysis result list is the same as that of the I<sup>2</sup>C bus signal analysis.

For the operating procedure, see section 1.5, "Saving the Data of the Detailed Analysis Result List."

#### Explanation

The data of the analysis result (simple display or detail display) to a specified storage medium in CSV format. The extension is .csv. Data in CSV format is a text file with data separated by commas. It is one of the common data formats used to convert data between spreadsheet and database applications.

#### Setting the Storage Conditions and Notes When Saving Data

The details are the same as when saving data of the analysis result list of the I<sup>2</sup>C bus signal. For details, see section 1.5.

#### Saved Data

Up to 3000 analysis results can be saved.

#### Data Size

Data size = (Number of frames + 4) × 155 [bytes]

\* The data size is a reference value. It is not strictly warranted. Use it as a guideline when saving the data.

#### Data Format

##### For the Detail display

Analysis Type SerialBus(CAN)  
Model Name DL9000  
Model Version \*.\*

No.	Frame	Time(ms)	ID	DLC	Hexadecimal display of DLC		Hexadecimal display of Data			Ack
					Binary display of Data	Hexadecimal display of Data	CRC	Hexadecimal display of the CRC sequence		
0	Data	-9.6091	00A(Hex)	2 Hex	00000001 Bin	01 Hex	A424 Hex	Y		
1	Data	-8.9693	012(Hex)	1 Hex	11111110 Bin	FE Hex	2263 Hex	Y		
2	Data	-9.3291	100(Hex)	3 Hex	11111111 Bin	FF Hex	6C6E Hex	Y		
3	Error	-7.6893			00000001 Bin	01 Hex				
					10100100 Bin	A4 Hex				
					00000001 Bin	01 Hex				

Analysis number: 0, 1, 2, 3  
 Frame type: Data, Error  
 Time from the trigger position to the head of the frame: -9.6091, -8.9693, -9.3291, -7.6893  
 ACK slot state: Y: ACK detected, N: ACK not detected

## 2.7 Error Messages

A message may appear on the screen during operation. This section describes the meanings of the messages and their corrective actions. This section lists only the error messages related to the CAN bus signal analysis function. There are other error messages related to the DL9000 and communications. These messages are described in the *User's Manual (IM701310-01E)* and the *Communication Interface User's Manual (IM701310-17E)*.

You can set the messages to be displayed in English or Japanese. For the procedure of setting the message language, see section 17.1, "Changing the Message Language and Turning ON/OFF the Click Sound" in the *User's Manual (IM701310-01E)*.

If the corrective action requires servicing, contact your nearest YOKOGAWA dealer for repairs.

Code	Message	Corrective Action	Page
58	Search execution is completed, but no record was found that matched the pattern.	–	2-25
506	Save data do not exist. Check the content to be saved.	Display the analysis result, and then execute the save operation again.	2-17, 2-32
670	The corresponding field was not found.	–	2-17

## 3.1 Overview of the SPI Bus Signal Analysis Function

### SPI Bus Signal Analysis Function

The SPI (Serial Peripheral Interface) Bus is a synchronized serial bus that is widely used for inter-IC communications and data communications.

By using this function, you will be able to analyze data while displaying the SPI Bus signal waveform.


The SPI Bus signal analysis function consists of the following three main functions.

#### Trigger Function <See page 3-5 for the operating procedure>

Acquires SPI Bus signals by comparing the specified conditions with the CH1 to CH4 input signals at the byte level (8 bits).

The data position to be compared can be specified in terms of the number of bytes from the assertion of the chip select signal (CS). You can set two data patterns (Data 1 and Data 2) for the four-wire SPI and one data pattern for the three-wire SPI. For Data 1 and Data 2, a trigger is activated at the position where the latter data pattern matches.

An example is given below for the case when comparing Data 1 (3 bytes) from the 4th byte after the assertion of the CS and comparing Data 2 (4 bytes) from the 10th byte after the assertion of the CS and activating the trigger when both patterns match

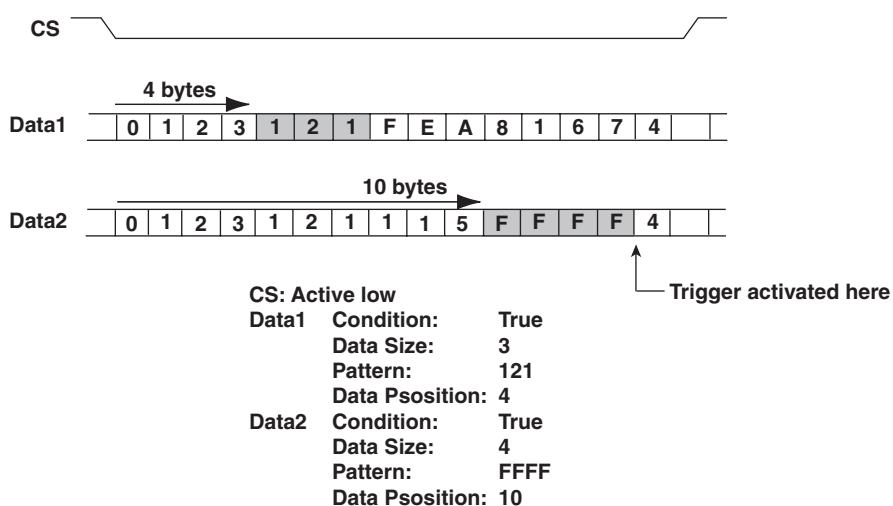


A trigger can be activated on the combination of the trigger conditions of the SPI bus signal and analog signal (event interval trigger). For details on the event interval trigger, see section 6.14 in the *User's Manual (IM701310-01E)*.

### 3.1 Overview of the SPI Bus Signal Analysis Function

#### Analysis Function <See pages 3-12 and 3-22 for the operating procedure>

This function analyzes the SPI bus signal data and shows a list of the analysis results. Analysis is performed at the byte level (8 bits) by synchronizing to the clock signal. There are two types of analysis result lists: simple and detail. The simple list displays the analysis number, Data 1/Data 2, and CS status for each byte. The detail list displays the time from the trigger position and the start and end positions of the active period in addition to the items displayed by the simple list. The data of the detail list can be saved to an arbitrary storage medium in CSV format. In addition, you can select an arbitrary byte in the analysis result list and move the zoom position (the center of the zoom box) to the head of that byte.

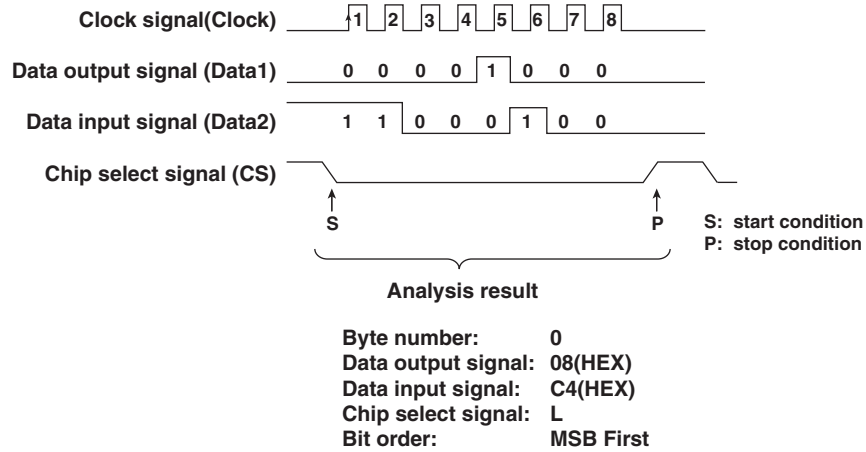

No.	Time(ms)	Data1(B)	Data1(H)	Data2(B)	Data2(H)	CS	S/P
80	0.336344	00000000	00	-----	--	H	
81	0.344344	00000000	00	-----	--	H	
82	0.352344	00000000	00	-----	--	H	
83	0.360344	00000000	00	-----	--	H	
84	0.368344	00000000	00	-----	--	H	
85	0.376344	00000000	00	-----	--	H	
86	0.384344	00000000	00	-----	--	H	P
87	0.400344	11000100	C4	-----	--	H	S P
88	0.424344	10101001	A9	-----	--	H	S
89	0.432344	00111011	3B	-----	--	H	P
90	0.472344	00000000	00	-----	--	H	S
91	0.480344	00000000	00	-----	--	H	
92	0.488344	00000000	00	-----	--	H	


#### Search Function <See page 3-21 for the operating procedure>

This function searches for data that matches or does not match a specific data pattern in the SPI bus signal data. When the search is executed, the zoom box moves to the data position where the conditions are met, and the data is displayed expanded in the zoom window (Zoom1 or Zoom2).

## 3.2 Setting the SPI Bus Signal Acquisition Conditions

The SPI Bus signal is acquired using the conditions of the SPI bus signal as trigger conditions.

### Procedure



- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Trigger Conditions of the SPI Bus Signal


1. Press **ENHANCED** to display the ENHANCED menu.
2. Press the **Type** soft key to display the Type menu.
3. Press the **SPI** soft key.

### Selecting Three-Wire or Four-Wire

4. Press the **Mode** soft key to select 3 wire or 4 wire.

### Selecting the Bit Order

5. Press the **Bit Order** soft key to set the read direction of the I/O data bits to MSB (MSB first) or LSB (LSB first).

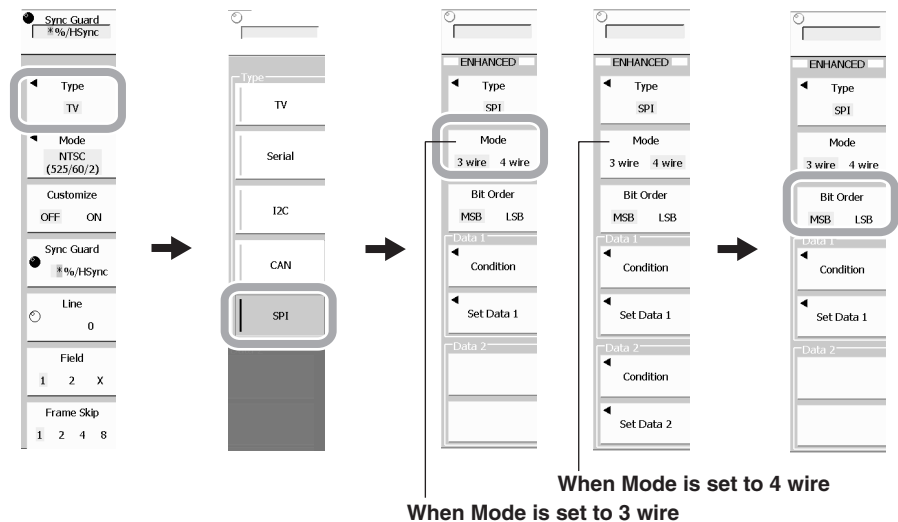


### 3.2 Setting the SPI Bus Signal Acquisition Conditions

#### Setting the Data Conditions

- **Setting the Conditions and Setting the Data Size**


6. Press the **Condition** soft key to display a menu used to set the condition and data size.
7. Press the **Condition** soft key to select True (match the specified bit pattern) or False (not match the specified bit pattern).
8. Press a soft key corresponding to the data size of the bit pattern (a trigger condition).
9. To activate a trigger the specified number of bytes after the assertion of the CS, use the **rotary knob** to set the trigger position (data position).

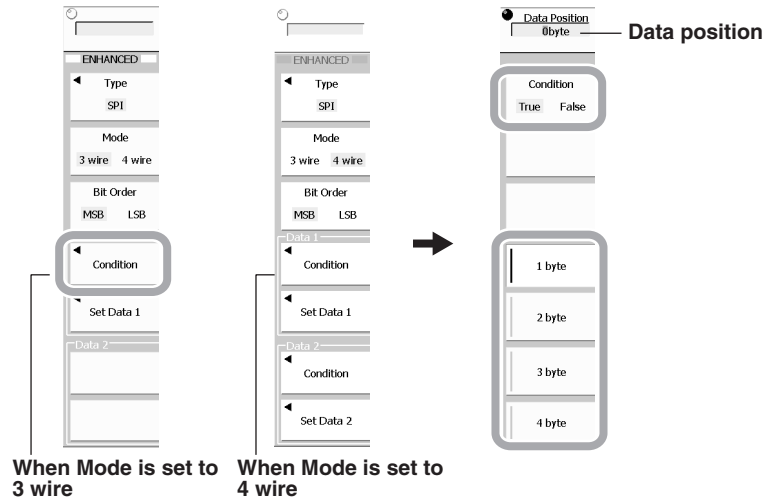

10. For four-wire, set the condition, data size, and data position for Data 2 in the same manner.
11. Press **ESC**.

- **Setting the Bit Pattern**

12. Press the **Set Data 1** soft key to display the bit pattern setting screen.
13. Turn the **rotary knob**, **arrow** keys, and **SET** key to set the pattern. You can use the soft keys to change the format to binary or hexadecimal or clear all the bits (X).

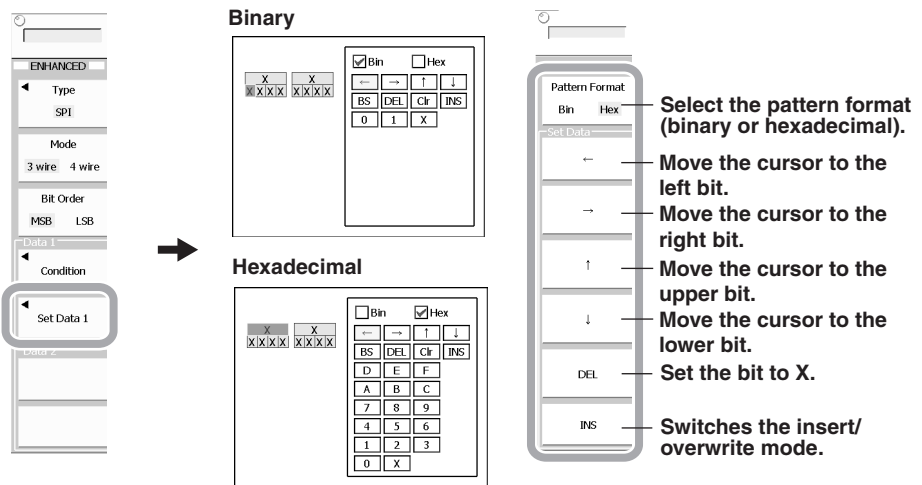

14. Press **ESC**.
15. For four-wire, set the bit pattern for Data 2 in the same manner.

**Setting the Source Channel**


16. Press **SOURCE** to display the SOURCE menu.

**Setting the CS**

17. Press the **Source** soft key under CS to display the CS source channel selection menu.
18. Press any of the soft keys **CH1** to **CH4** to assign the channel to the CS.
19. Press the **Active** soft key to select H (high) or L (low).


**Setting the Clock**

20. Press the **Source** soft key under Clock to display the clock source channel selection menu.
21. Press any of the soft keys **CH1** to **CH4** to assign the channel to the clock channel.
22. Press the **Polarity** soft key to select rising or falling.

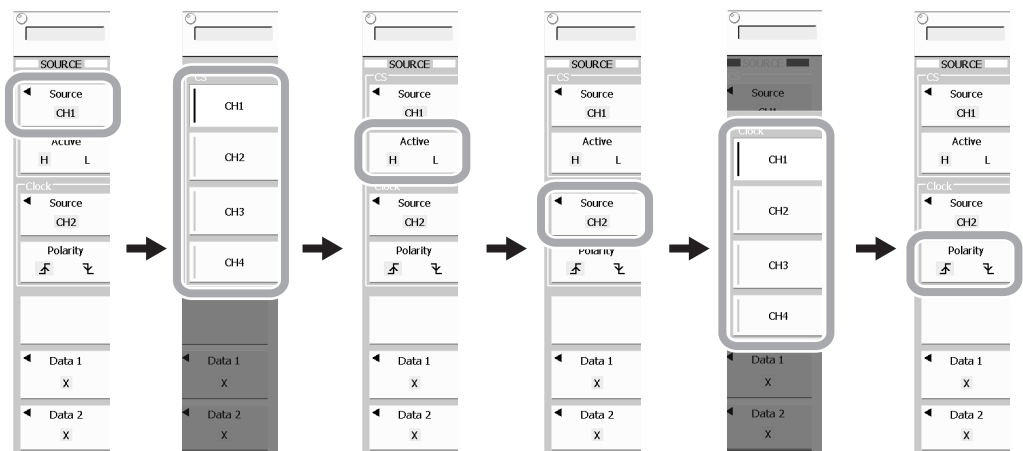

**Select the Channel for Comparing the Bit Pattern**

23. Press the **Data 1** soft key to display a menu used to select the channel to compare to the bit pattern of Data 1.
24. Press any of the soft keys, **CH1** to **CH4**.
25. For four-wire, select the channel for comparing the bit pattern for Data 2 in the same manner.

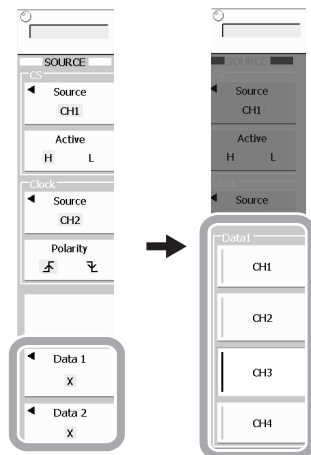



## 3.2 Setting the SPI Bus Signal Acquisition Conditions

### Setting the Level, Coupling, HF Rejection, and Hysteresis

26. Press **LEVEL/COUPLING** to display the LEVEL/COUPLING menu.

#### Selecting the Channel to Be Configured

27. Press the **CH** soft key to display a channel selection menu.
28. Press any of the soft keys, **CH1** to **CH4**.

#### Setting the Level

29. Turn the **rotary knob** to set the level used to determine high/low. The level is common to all channels.

#### Setting the Coupling


30. Press the **Coupling** soft key to select DC.

#### Setting the HF Rejection

31. Press the **HF Rejection** soft key to display a HF rejection selection menu.
32. Press any of the soft keys, **OFF**, **20MHz**, or **15kHz**.

#### Setting the Hysteresis

33. Press the **Hysteresis** soft key to select the hysteresis.

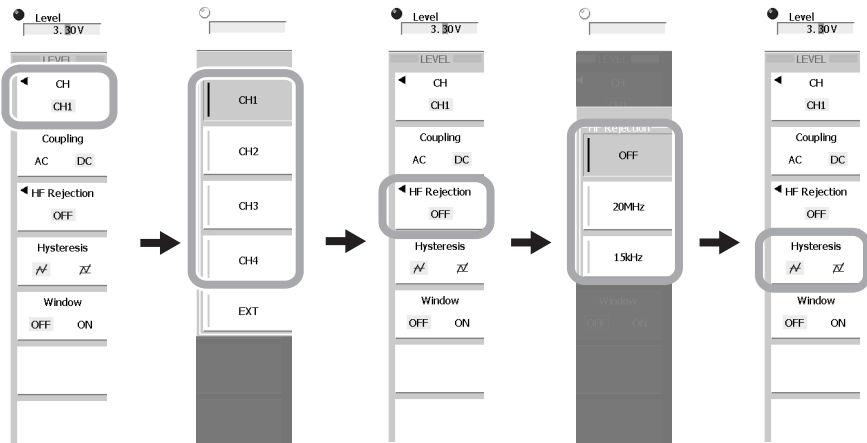

As necessary, repeat steps 27 to 33.

**Explanation****Setting the Trigger Conditions of the SPI Bus Signal****Three-Wire or Four-Wire (Mode)**

For three-wire, triggers are activated on the Data 1 bit pattern.

For four-wire, triggers are activated on the Data 1 and Data 2 bit patterns. The Data 1 and Data 2 data patterns can also be used as independent trigger conditions.

**Bit Order**

You can select the bit order of Pattern A and Pattern B according to the signal flow of the input/output data.

MSB	Select this when the I/O data signal is flowing MSB first.
LSB	Select this when the I/O data signal is flowing LSB first.

**Data Conditions**

- **Condition**

You can select either of the following:

True	A trigger is activated when the data matches the specified bit pattern.
False	A trigger is activated when the data does not match the specified bit pattern.

- **Data Size**

Select the number of bytes (data length) of bit pattern to be specified in the range of 1 to 4 bytes.

- **Data Position**

Compares the pattern the specified number of bytes after the assertion of the chip select (CS). The data position can be set separately for Data 1 and Data 2. The selectable range is 0 to 9999.

- **Pattern Format**

Set the bit pattern format to either of the following:

Hex	Hexadecimal
Bin	Binary

- **Bit Pattern**

Set the bit pattern. When Pattern Format is set to Hex (hexadecimal), you can enter X, 0 to 9, or A to F in units of 4 bits. When Pattern Format is set to Bin (binary), you can enter X, 0, or 1 for each bit.

**Source Channel**

The source channel of the SPI bus signal is set using the SOURCE menu that appears when you press the SOURCE key. The menu used to set the source channel of the SPI bus signal appears only when Type is set to SPI in the ENHANCED menu.

**Chip Select (CS)**

Select the CS from CH1 to CH4. Select whether to make the signal active when it is high or low with the Active item.

**Clock Signal**

Select the input signal to be the clock signal from CH1 to CH4.  
The bit pattern is compared on the rising or falling edge of the signal.

**Channel for Comparing the Bit Pattern (Data1/Data2)**

Select the signal for comparing the bit pattern from CH1 to CH4.

**Trigger Level, Trigger Coupling, Etc.**

Set the trigger level, hysteresis, trigger coupling, and HF rejection of each channel. For details on these items, see the *User's Manual (IM701310-01E)*.

### 3.2 Setting the SPI Bus Signal Acquisition Conditions

#### Unification of the Trigger Setting of the SPI Bus Signal and the Setting of the SPI Bus Signal Analysis and Search

On products with software version 1.80 or higher, the trigger settings of the SPI bus signal on the menu that is entered through the ENHANCED key and the settings of the SPI bus signal analysis and search on the menu entered through the WINDOW1 and ZOOM1 key are common. The CH1 to CH4 sources are the waveforms of which the settings are common.

#### Trigger settings of the SPI bus signal that are applied to the settings of both the SPI bus signal analysis and search

Level (trigger level), Hysteresis (trigger hysteresis)  
 (The settings of the SPI bus signal analysis and search are not applied to the trigger settings of the SPI bus signal.)

#### Item of which the trigger settings of the SPI bus signal, the settings of the SPI bus signal analysis, and the settings of the SPI bus signal search that are mutually applied


Mode, Bit Order, CS Source, CS Active, Clock Source, Clock Polarity, Data1, Data2

#### Note

- M1 to M4 does not apply to the common settings.
- The settings of the SPI bus signal analysis and search on the menu entered through the WINDOW2 and ZOOM2 keys are not made common. They are independent settings.
- If you change common items (excluding Level and Hys) in the analysis and search menus while the waveform acquisition is in progress and the trigger type is set to SPI, the waveform acquisition is restarted.
- Even if something other than SPI bus is selected in the analysis or search menu, the level and hysteresis settings of the analysis and search are set to the same value if the trigger level or hysteresis setting is changed.
- When the trigger level or hysteresis is changed by executing auto setup, the level and hysteresis settings of the analysis and hysteresis are also set to the same new value. This also applies when the setup information is initialized.
- Trigger hysteresis  $\swarrow$  and  $\searrow$  correspond to 0.6 division and 1.0 division, respectively, of the analysis or search.

#### Examples of SPI Bus Signal Trigger Conditions


The trigger point is set to the position indicated below depending on the clock edge slope setting (see page 3-5).

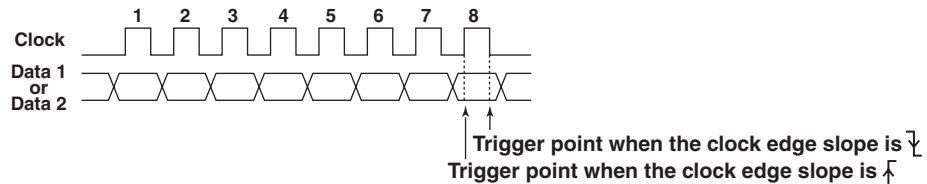

This section will indicate the data sequence at the byte level in hexadecimal and indicate the position where the trigger will occur. The shaded section in the figure indicates the byte pattern (sequence) that is compared. We assume that CH1 is selected for comparing the bit pattern of Data 1 and CH2 is selected for comparing that of Data 2.

#### Trigger Conditions


CS	L
Data 1	A4 25
Data Byte Condition	2
Byte Position	True
	0
Data 2	85 C8
Data Byte Condition	2
Byte Position	True
	6

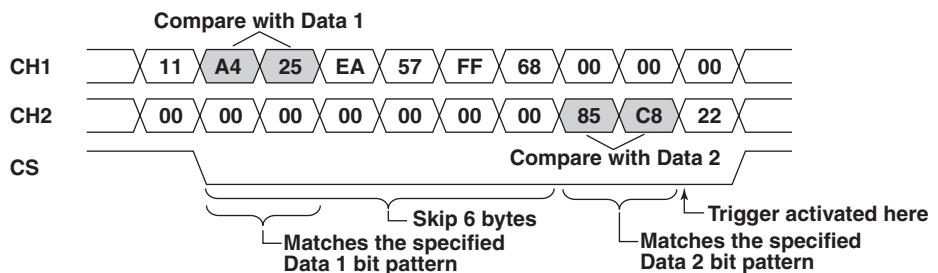

## 3.3 Analyzing the Data

By setting analysis conditions, the SPI signal data stored to the acquisition memory can be analyzed.



### Procedure

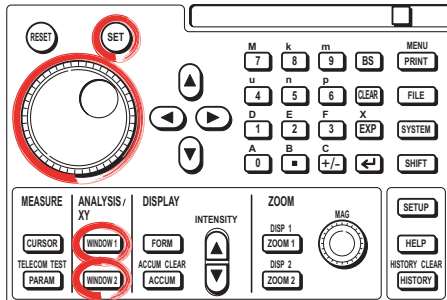

- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.


### Setting the Analysis Conditions

1. Press **WINDOW1** or **WINDOW2**.
2. Press the **Type** soft key to display the Type menu.
3. Press the **Serial Bus** soft key.
4. Press the **Analyze** soft key to display the Analyze menu.
5. Press the **Mode** soft key to display the Mode menu.
6. Press the **SPI** soft key.

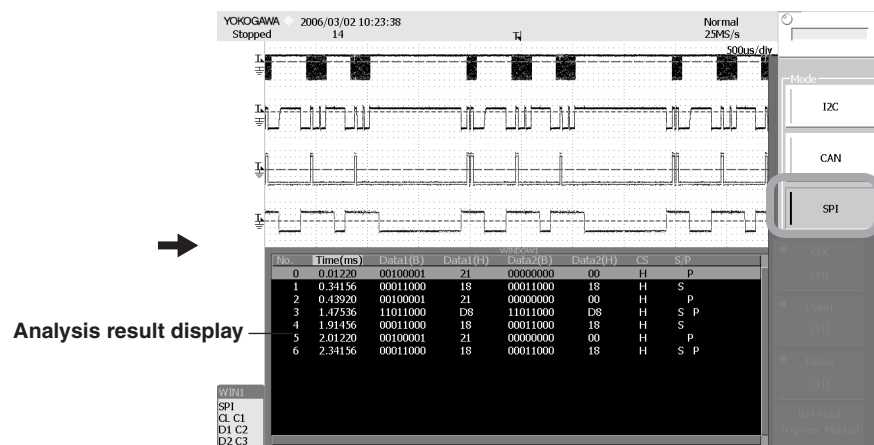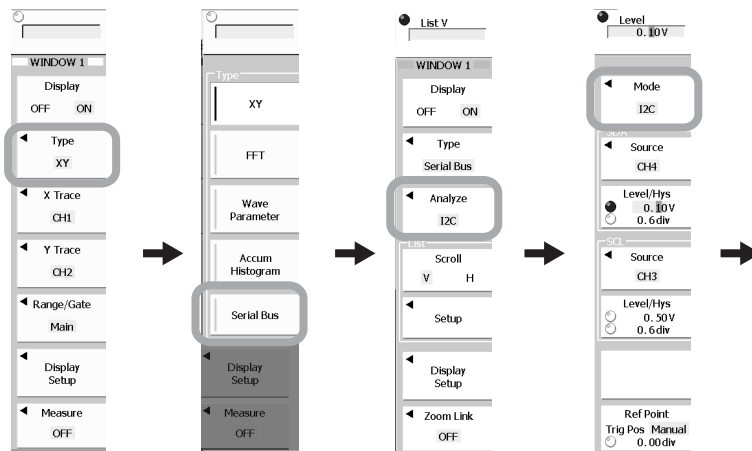

#### Selecting Three-Wire or Four-Wire and Selecting the Bit Order


7. Press the **Setup** soft key to display a menu used to set three-wire or four-wire.
8. Press the **Mode** soft key to select 3 wire or 4 wire.
9. Press the **Bit Order** soft key to set the read direction of the I/O data bits to MSB or LSB.

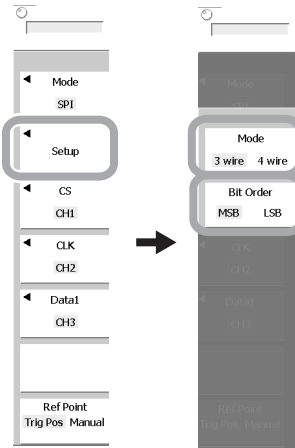

10. Press **ESC**.

#### Setting the Chip Select Signal (CS)


11. Press the **CS** soft key to display the CS menu.
12. Press the soft key corresponding to the channel to be assigned to CS.
13. Press the **Active** soft key to set the CS enable status to H (high) or L (low).
14. Press the **Level/Hys** soft key to move the cursor to the level value.
15. Turn the **rotary knob** to set the level for determining the status of the CS signal.
16. Press the **Level/Hys** soft key to move the cursor to the hysteresis value.
17. Turn the **rotary knob** to set the hysteresis.

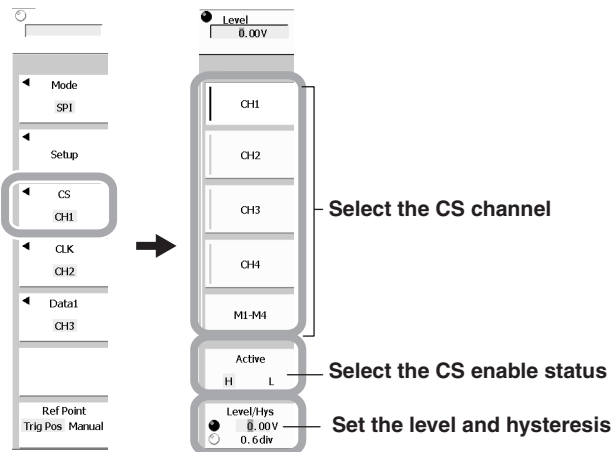

18. Press **ESC**.

**Setting the Clock Signal (CLK)**


19. Press the **CLK** soft key to display the CLK menu.
20. Press the soft key corresponding to the channel to be assigned to the clock signal.
21. Press the **Polarity** soft key to select rising (↗) or falling (↘).
22. Press the **Level/Hys** soft key to move the cursor to the level value.
23. Turn the **rotary knob** to set the level used to determine the rising or falling edge of the clock signal.
24. Press the **Level/Hys** soft key to move the cursor to the hysteresis value.
25. Turn the **rotary knob** to set the hysteresis.

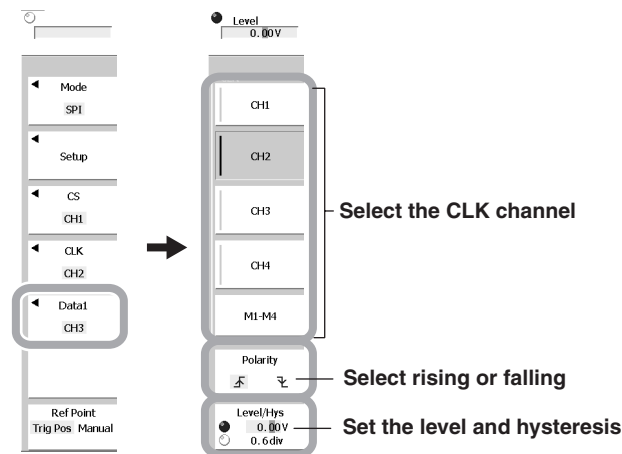

26. Press **ESC**.

**Setting Data 1 (Data 2)**


27. Press the **Data 1** or **Data 2** soft key (for four-wire) to display the Data 1 or Data 2 menu.
28. Press the soft key corresponding to the channel to be assigned to Data 1 or Data 2.
29. Press the **Active** soft key to set H or L. If set to H, the signal is determined to be 1 when the level for determining the status is exceeded and 0 otherwise. If set to L, the signal is determined to be 1 when the level for determining the status is not exceeded and 0 otherwise.
30. Press the **Level/Hys** soft key to move the cursor to the level value.
31. Turn the **rotary knob** to set the level used to determine status.
32. Press the **Level/Hys** soft key to move the cursor to the hysteresis value.
33. Turn the **rotary knob** to set the hysteresis.

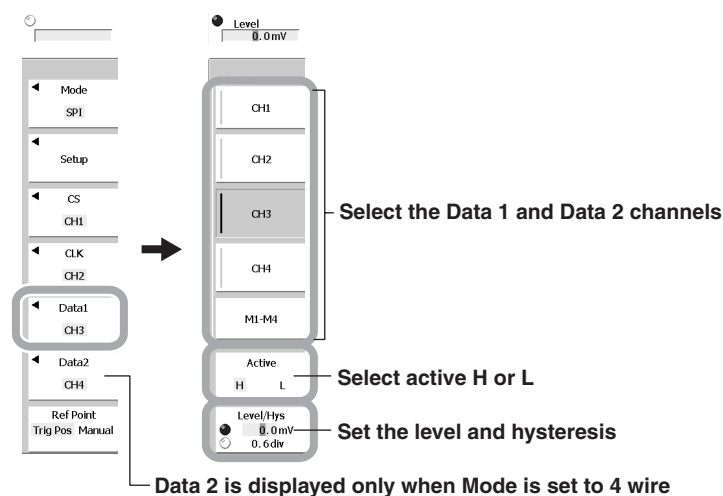

34. Press **ESC**.


#### Setting the Analysis Reference Point

35. Pressing the **Ref Point** soft key to select Trig Pos or Manual.  
If you selected Manual, turn the rotary knob to set the reference point in the range of  $\pm 5.00$  divisions.

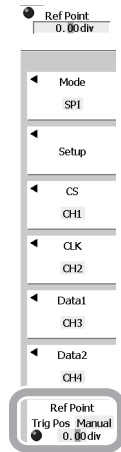

#### Display the Analysis Results

36. Press the **ESC**.
37. Press the **Scroll** soft key to select V (scroll vertically) or H (scroll horizontally).
38. Press the **Setup** soft key to display a menu used to set the analysis display.
39. Press the **Mode** soft key to select Simple (simple display) or Detail (detailed display).
40. Press any of the soft keys **1**, **10**, **100**, **1000**, and **10000** to set the step number for scrolling.
41. Press **ESC**.
42. Press the **Display Setup** soft key to display the Display Setup menu.
43. Press the **VT** soft key to select ON or OFF. If ON is specified, the waveform is displayed on a normal voltage-time axis.
44. Press the **ESC**.

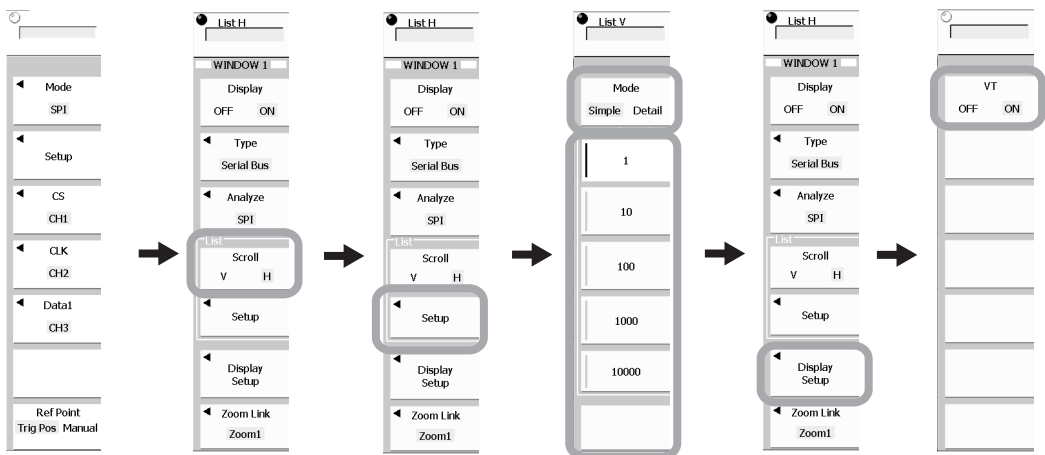


#### Note

The detailed analysis list can be saved directly to a storage medium in CSV format (.csv extension). For details, see section 3.5.

### Zoom Link

45. Press the **Zoom Link** soft key to display the Zoom Link menu.
46. Press any of the soft keys, **OFF**, **Zoom1**, or **Zoom2** to set the link to the zoom screen. The zoom position (the center of the zoom box) can be moved to the head of the byte selected in the analysis result list by linking Zoom1 or Zoom2.

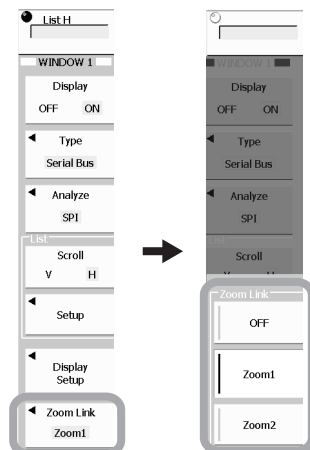

### Explanation

#### Setting the Analysis Conditions

You can set the following conditions.

##### Three-Wire or Four-Wire

Select three-wire SPI or four-wire SPI. One type of data (Data 1) can be analyzed for three-wire SPI and two types of data (Data 1 and Data 2) for four-wire SPI.

##### Read Direction of the I/O Data Bits (Bit Order)

You can select the read direction of the bits according to the signal flow.

MSB First	Select this when the I/O data signal is flowing MSB first.
LSB First	Select this when the I/O data signal is flowing LSB first.



##### Chip Select Signal (CS (SS))

You can select CH1 to CH4 or M1 to M4 signals for the CS signal on the SPI bus.

- **Level**

When the channel signal is set to be the CS signal, you can set the level for determining the high (H) or low (L) status of the CS signal for each channel.

Selectable range:  $\pm 10$  divisions around the vertical position

Resolution: 0.01 divisions (For example, the resolution for 2 mV/div is 0.02 mV.)

- **Hysteresis**

Selectable range: 0.0 division to 4.0 divisions

Resolution: 0.1 divisions

- **Enable Status of the CS Signal (Active)**

You can select the enable status of the CS signal. The setting applies to all CS signals.

H Analyzes the I/O data when the CS signal is higher than the level for determining the status.

L Analyzes the I/O data when the CS signal is less than the level for determining the status.



#### Clock Signal

Set the channel to which the clock signal on the SPI Bus is being applied. The status of the I/O data is determined by synchronizing to the clock signal. You can set the detection level, slope, and hysteresis of the clock signal.

- **Level**

You can set the level\* for detecting the synchronization clock.

Selectable range:  $\pm 10$  divisions around the vertical position

Resolution: 0.01 divisions (For example, the resolution for 2 mV/div is 0.02 mV.)

- **Hysteresis**

You can set the hysteresis\* on the level for detecting the synchronization clock.

Selectable range: 0.0 division to 4.0 divisions

Resolution: 0.1 divisions


- **\* Detecting the Synchronization Clock**

- When the level of the clock signal changes from below the specified lower limit of hysteresis to above and including the upper limit of hysteresis, it is detected as a synchronization clock.
- When the level of the clock signal changes from above the specified upper limit of hysteresis to below and including the lower limit of hysteresis, it is detected as a synchronization clock.
- For all other cases, it is not detected as a synchronization clock.


- **Slope (Polarity)**

You can select which slope edge, rising or falling, of the synchronization clock is to be detected.

---

 Rising slope

---

 Falling slope

---

#### Analyzed Data (Data 1 and Data 2)

The data below can be analyzed for the I/O data signal (Data 1 and Data 2) on the SPI bus.

- **Waveform Data**

Analysis can be performed regardless of whether the waveform acquisition is in progress. If the waveform acquisition is in progress, the analysis results are updated in real-time in sync with the displayed waveform. The waveform data stored in the history memory (waveform data of the record number selected using HISTORY menu > Select) is also analyzed.

- **Loaded Acquisition Data (ACQ data)**

- **Condition for Determining the Status (Active)**

Set the condition for determining 1 or 0.

---

H Determines that the status is 1 when the signal is greater than or equal to the level for determining the status or 0 otherwise.

---

L Determines that the status is 1 when the signal is less than or equal to the level for determining the status or 0 otherwise.

---

- **Level**

You can set the level\* for determining the status of the data to be analyzed.

Selectable range:  $\pm 10$  divisions around the vertical position

Resolution: 0.01 divisions (For example, the resolution for 2 mV/div is 0.02 mV.)

- **Hysteresis**

You can set a hysteresis\* on the level for determining the status of the data to be analyzed.

Selectable range: 0.0 division to 4.0 divisions

Resolution: 0.1 divisions

- **\* Determining 1 and 0 of the Analyzed Data**

- **When Active Is Set to H**

When the level of the analyzed data changes from below the hysteresis lower limit to greater than or equal to the hysteresis upper limit, the data is determined to be 1. When the level of the analyzed data changes from above the hysteresis upper limit to less than or equal to the hysteresis lower limit, the data is determined to be 0.

- **When Active Is Set to L**


When the level of the analyzed data changes from above the hysteresis upper limit to less than or equal to the hysteresis lower limit, the data is determined to be 1. When the level of the analyzed data changes from below the hysteresis lower limit to greater than or equal to the hysteresis upper limit, the data is determined to be 0.

**Analysis Reference Point (Ref Point)**

Select the analysis reference point from below.

Trig Pos	Sets the trigger position to the analysis reference point.
Manual	Manually set the analysis reference point. Selectable range: $\pm 5.00$ divisions, resolution: 0.01 divisions

Depending on the analysis reference point (Ref Point), the No. 0 byte in the analysis result list is as follows:



- (A): No. 0 byte -> Byte 1 (Byte 2 is No. 1, byte 3 is No. 2, ...)
  - (B): No. 0 byte -> Byte 1 (Byte 2 is No. 1, byte 3 is No. 2, ...)
  - (C): No. 0 byte -> Byte 2 (byte 1 is No. -1, byte 3 is No. 1, byte 4 is No. 2...)
  - (D): No. 0 byte -> Byte 5 (byte 1 is No. -4, ... byte 4 is No. -1, byte 6 is No. 1...)
- S: Start condition, P: Stop condition

**Unification of the Trigger Setting of the SPI Bus Signal and the Setting of the SPI Bus Signal Analysis and Search**

On products with software version 1.80 or higher, the trigger settings of the SPI bus signal on the menu that is entered through the ENHANCED key and the settings of the SPI bus signal analysis and search on the menu entered through the WINDOW1 and ZOOM1 key are common. For details, see page 3-7.

**Analysis Range**

Up to 40000 bytes of analysis data can be displayed.

**Analysis Data List (Analysis Result List)**

The following items are displayed.

**Simple Display**

- Analysis number (No.): Up to 40000 points can be displayed.
- Hexadecimal display of the Data 1 (Data 1(H))
- Hexadecimal display of the Data 2 (Data 2(H))
- CS status


Analysis number  
Data 1 value (Hexadecimal)  
Data 2 value (Hexadecimal)  
CS status

No.	Data1(H)	Data2(H)	CS
80	00	--	H
81	00	--	H
82	00	--	H
83	00	--	H
84	00	--	H
85	00	--	H
86	00	--	H
87	C4	--	H
88	A9	--	H
89	3B	--	H
90	00	--	H
91	00	--	H
92	00	--	H

### 3.3 Analyzing the Data

#### Detail Display

- Analysis number (No.): Up to 40000 points can be displayed.
- Time from the trigger position to the start bit of each data (Time(ms))
- Binary display of the Data 1 (Data 1(B))
- Hexadecimal display of the Data 1 (Data 1(H))
- Binary display of the Data 2 (Data 2(B))
- Hexadecimal display of the Data 2 (Data 2(H))
- CS status
- Start/Stop position of the active period (S/P)

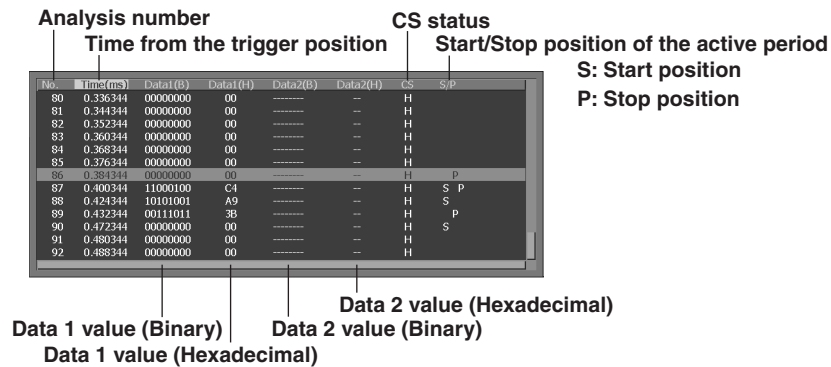

#### Zoom Link


Select from the following:

OFF	Disables the zoom link function.
Zoom1	Links to Zoom1.
Zoom2	Links to Zoom2.

By default, WINDOW1 and WINDOW2 are linked to Zoom1 and Zoom2, respectively. If Zoom1 or Zoom2 is selected and you select (highlight) an arbitrary byte in the analysis result list, the zoom position (the center of the zoom box) of Zoom1 or Zoom2 moves to the head of that byte. Conversely, if you change the zoom position of Zoom1 or Zoom2, the highlight in the analysis result list moves to the byte that is shown in the zoom box of Zoom1 or Zoom2.

#### Display Example of Analysis Data

Examples of analysis using different analysis conditions are indicated below.

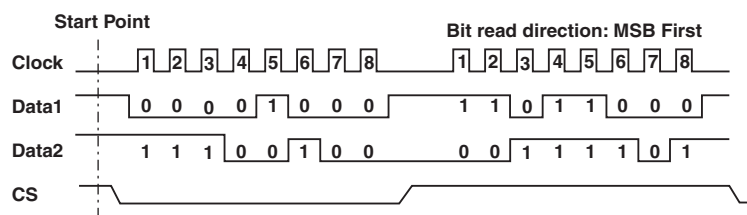

- **Analysis Condition Clock (CH1) =  $\bar{f}$  and CS (CH4) = L**

Display Item	Analysis Data Display
Analysis number (No.)	0
Hexadecimal display of Data1 (Dt1)	08
Hexadecimal display of Data2 (Dt2)	E4
Status of the CS signal (CS)	L

- **Analysis Condition Clock (CH1) =  $\bar{f}$  and CS (CH4) = H**

Display Item	Analysis Data Display
Analysis number (No.)	0
Hexadecimal display of Data1 (Dt1)	D8
Hexadecimal display of Data2 (Dt2)	3D
Status of the CS signal (CS)	H


#### Note

If the CS signal is ON and the CS signal on the main waveform display screen does not contain a transition point from H to L or L to H, the I/O data is not analyzed.

## 3.4 Searching the Waveform

You can search waveforms that match the specified conditions among the acquired waveforms. The search conditions are the same as the trigger settings of section 3.2.


### Procedure

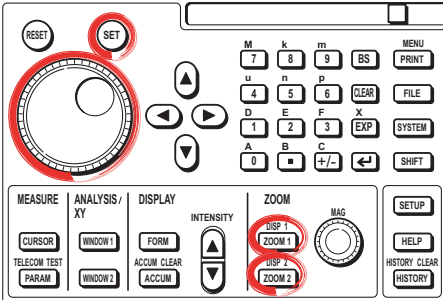


- To exit the menu during operation, press **ESC** located above the soft keys.
- For details on the operation using the rotary knob, SET, and RESET, see sections 4.1 or 4.2 in the *User's Manual (IM701310-01E)*.
- For a description of the operation using a USB keyboard or a USB mouse, see section 4.3 in the *User's Manual (IM701310-01E)*.

### Setting the Search Conditions

1. Press **ZOOM1** or **ZOOM2** to display the ZOOM menu.
2. Press the **Setup** soft key to display the search condition menu.
3. Press the **Search Type** soft key.
4. Press the **Serial** soft key.
5. Press the **SPI** soft key.
6. Press the **Setup** soft key to display the search condition menu.

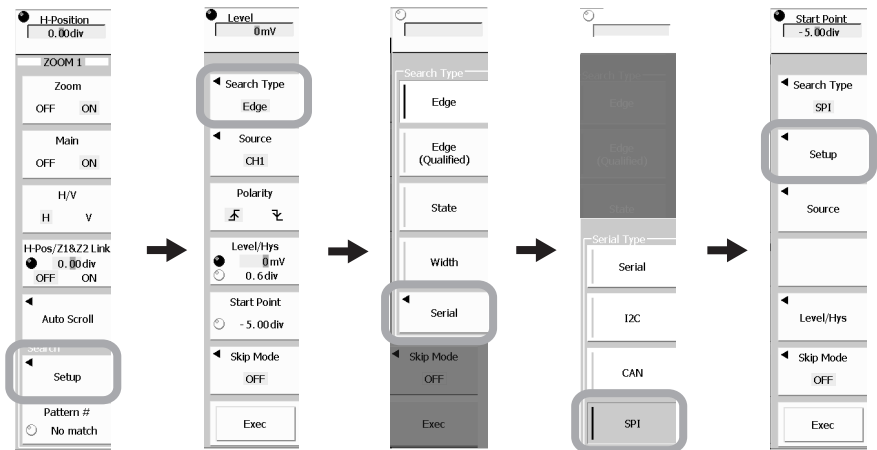

The procedure of setting the search conditions are the same as the trigger conditions. See page 2-6 (the position of the soft keys may be different).

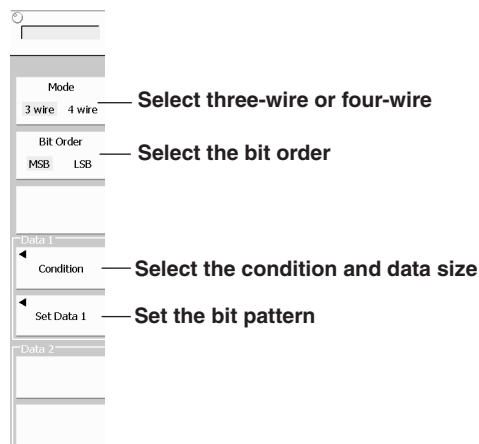


### Setting the Source Channel

7. Press the **Source** soft key to display the source channel menu.


### Setting the CS

8. Press the **Source** soft key under CS to display the CS source channel selection menu.
9. Press the soft key corresponding to the channel to assign to CS.
10. Press the **Active** soft key to set the CS enable status to H (high) or L (low).

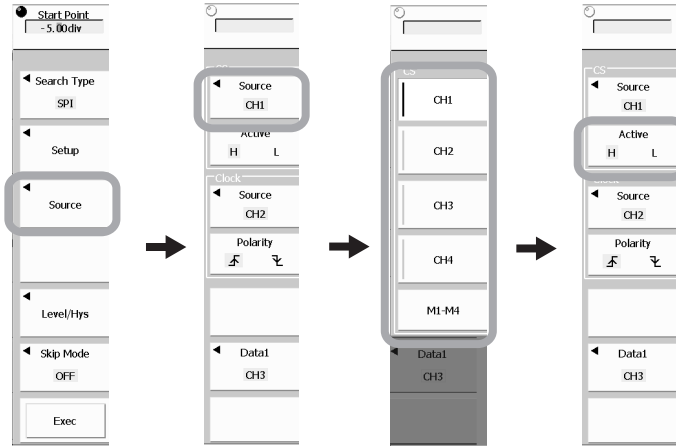


### Setting the Clock

11. Press the **Source** soft key under Clock to display the Clock source channel selection menu.
12. Press the soft key corresponding to the channel to assign to the clock signal.
13. Press the **Polarity** soft key to select rising ( $\uparrow$ ) or falling ( $\downarrow$ ).

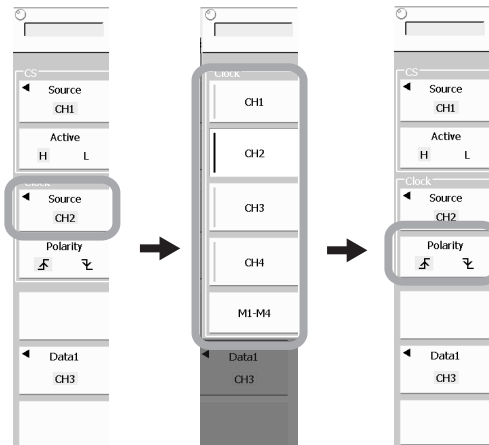

**Setting Data 1 (Data 2)**

14. Press the **Data1** or **Data2** soft key (for four-wire) to display a menu used to select the Data1 or Data2 channels.
15. Press the soft key corresponding to the channel to be assigned to Data1 or Data2.

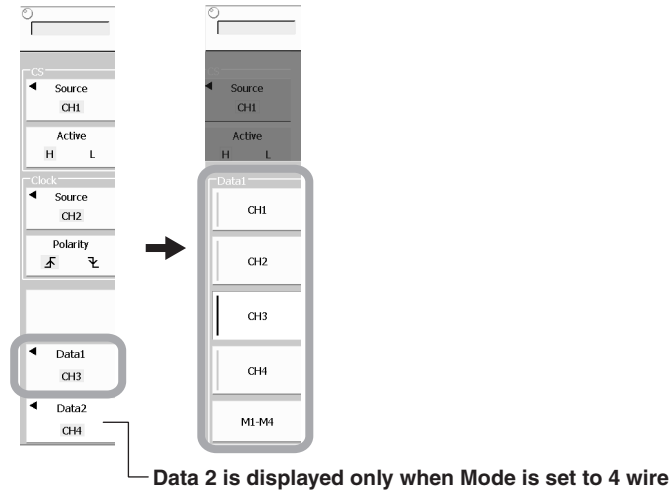


16. Press **ESC** to return to the previous screen.

**Setting the Level and Hysteresis**

17. Press the **Level/Hys** soft key.
18. Press the soft key corresponding to the channel you wish to configure.
19. Turn the **rotary knob** to set the level or hysteresis.
20. Press **ESC**.

**Setting the Skip Mode**

21. Set the skip mode as necessary.  
Press the **Skip Mode** soft key to display the skip mode menu.
22. Press the **OFF**, **Hold Off**, or **Decimation** soft key.
23. Turn the **rotary knob** to set the time to skip or the search count.
24. Press **ESC**.

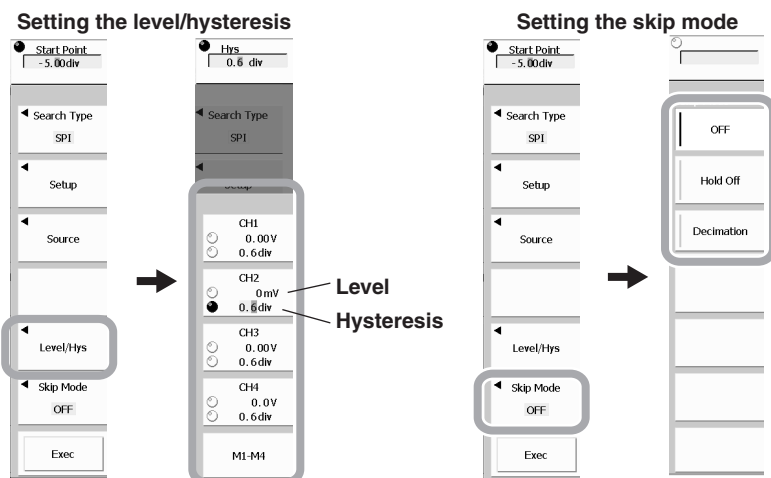

### 3.4 Searching the Waveform

#### Setting the Search Start Point


- Turn the **rotary knob** to set the Start Point.

#### Executing the Search

- Press the **Exec** soft key. The section that meets the search conditions is shown on the ZOOM display.

#### Viewing Search Points

- Press **ESC**.
- Press the **Pattern #** soft key.
- Turn the **rotary knob** to select an arbitrary search point. The zoom position moves to the selected search point.

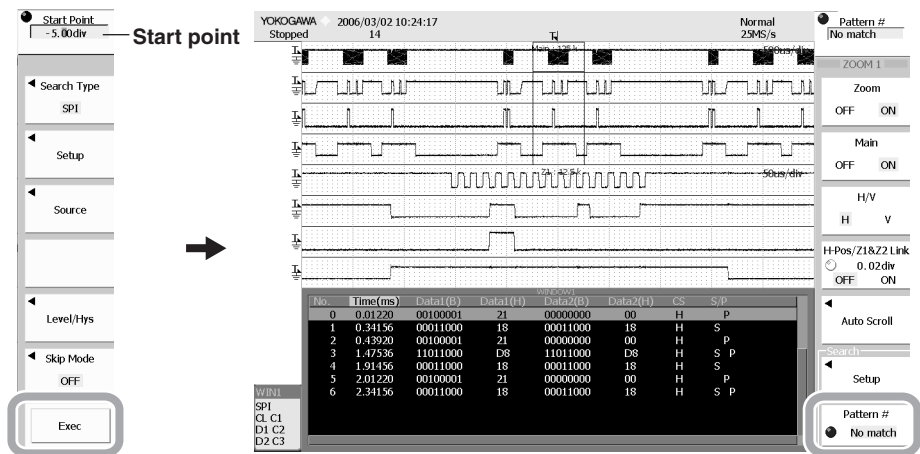

#### Explanation

#### Setting the Search Conditions

You can set the following conditions.

- Three-wire or four-wire
- Bit Order
- Condition and bit pattern of Data 1 and Data 2

The search conditions are the same as the trigger conditions. For details, see section 3.2.

#### Source Channel, Qualification, Level, Hysteresis, Etc.

The settings for the source channel, qualification, trigger level, trigger coupling, and so on are the same as the settings of the analysis conditions. For details, see section 3.3.

#### Skip Mode

After searching the position that meets the search conditions, the specified amount of time or the number of positions that match the search conditions are skipped.


OFF	Searches all sections that meet the search conditions.
Hold Off	Skips the search for the specified time.
Decimation	Skips the specified number of search positions.

#### Search Start Point

Set the position to start the search in the range of  $\pm 5.00$  divisions.

### Search Point

When the search is executed, the zoom box (ZOOM1 or ZOOM2) moves to the data position where the conditions are met. The search point is the center of this zoom box. The search point is set to the same position as the trigger position (see page 3-8).

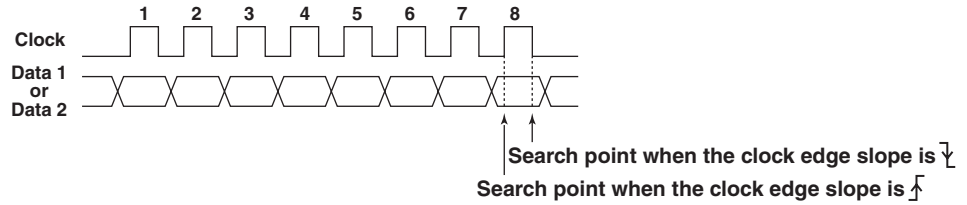

### Viewing Search Points

If you select an arbitrary search point using Pattern #, the zoom position moves to the selected search point. If the zoom link function is enabled (see page 3-16), the highlight in the analysis result list also moves to the byte containing the selected search point.

### Unification of the Trigger Setting of the SPI Bus Signal and the Setting of the SPI Bus Signal Analysis and Search

On products with software version 1.80 or higher, the trigger settings of the SPI bus signal on the menu that is entered through the ENHANCED key and the settings of the SPI bus signal analysis and search on the menu entered through the WINDOW1 and ZOOM1 key are common. For details, see page 3-7.



## 3.5 Saving the Data of the Analysis Result List

### CAUTION

Do not remove the medium (disk) or turn OFF the power when the access indicator is blinking. Doing so can damage the storage medium or destroy the data on the medium.

#### Procedure

The procedure to save the results is the same as with the I<sup>2</sup>C Bus signal analysis. For the operating procedure, see section 1.5, "Saving the Data of the Detailed Analysis List."

#### Explanation

The analysis results can be saved in CSV format to a specified storage medium. The extension is .csv. Data in CSV format is a text file with data separated by commas. It is one of the common data formats used to convert data between spreadsheet and database applications.

#### Setting the Storage Conditions and Notes When Saving Data

The details are the same as when saving data of the analysis result list of the I<sup>2</sup>C bus signal. For details, see section 1.5.

#### Saved Data

Up to 40000 analysis results in the past from the point when the save operation was executed can be saved.

#### Data Size

Data size\* = (Number of bytes + 4) × 79 [bytes]

\* The data size is a reference value. It is not strictly warranted. Use it as a guideline when saving the data.

#### Data Format

No.	Time(ms)	Binary display of Data1		Hexadecimal display of Data1		Binary display of Data2		Hexadecimal display of Data2		CS status	
		Data1(B)	Data1(H)	Data2(B)	Data2(H)	CS	S/P				
0	-0.68336	00011110 Bin	1E Hex	11110111 Bin	F7 Hex	L	S	P			
1	-0.66736	10111101 Bin	BD Hex	01111111 Bin	7F Hex	L	S				
2	-0.65936	01000010 Bin	42 Hex	11010100 Bin	D4 Hex	L		P			
3	-0.63536	10010011 Bin	93 Hex	11100111 Bin	E7 Hex	L	S				
4	-0.62736	10111101 Bin	BD Hex	11111111 Bin	FF Hex	L					
5	-0.61936	01000010 Bin	42 Hex	11111111 Bin	FF Hex	L					
6	-0.61136	10001100 Bin	8C Hex	01111111 Bin	7F Hex	L		P			

Analysis SerialBus(SPI)  
Model NarDL9000  
Model Ver\*,\*\*

Time from the start point  
Analysis number

CS active start (S)/stop (P)

## 3.6 Error Messages

A message may appear during operation. This section describes the meanings of the messages and their corrective actions. This section lists only the error messages related to the SPI Bus signal analysis function. There are other error messages related to the DL9000 and communications. These messages are described in the *User's Manual (IM701310-01E)* and the *Communication Interface User's Manual (IM701310-17E)*. You can set the messages to be displayed in English or Japanese. For the procedure of setting the message language, see section 17.1, "Changing the Message Language and Turning ON/OFF the Click Sound" in the *User's Manual (IM701310-01E)*. If the corrective action requires servicing, contact your nearest YOKOGAWA dealer for repairs.

Code	Messages	Corrective Action	Page
58	Search executed is completed, but no record was found that matched the pattern.	–	3-17
506	Save data do not exist. Check the content to be saved.	Display the analysis result, and then execute the save operation again.	3-9, 3-22

## 4.1 A List of Commands

### ANALysis Group

Command	Function	Page
:ANALysis:SBUS<x>?	Queries all settings related to the serial bus signal analysis function.	4-15
:ANALysis:SBUS<x>:ANALyze?	Queries all settings related to the serial bus signal analysis.	4-15
:ANALysis:SBUS<x>[:ANALyze]:CANBus?	Queries all settings related to the CAN bus signal analysis.	4-15
:ANALysis:SBUS<x>[:ANALyze]:CANBus:BRATe	Sets the bit rate (data transfer rate) of the CAN bus signal analysis or queries the current setting.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:FJUMp:ACK	Executes a field jump to the ACK Field in the results of the CAN bus signal analysis.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:FJUMp:CONTRol	Executes a field jump to the Control Field in the results of the CAN bus signal analysis.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:FJUMp:CRc	Executes a field jump to the CRC Field in the results of the CAN bus signal analysis.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:FJUMp:DATA	Executes a field jump to the Data Field in the results of the CAN bus signal analysis.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:FJUMp:IDENtifier	Executes a field jump to the Identifier Field in the results of the CAN bus signal analysis.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:FJUMp:SOF	Executes a field jump to the SOF Field in the results of the CAN bus signal analysis.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:REcEssive	Sets the recessive level (bus level) of the CAN bus signal analysis or queries the current setting.	4-16
:ANALysis:SBUS<x>[:ANALyze]:CANBus:SPOint	Sets the sample point of the CAN bus signal analysis or queries the current setting.	4-17
:ANALysis:SBUS<x>[:ANALyze]:CANBus:TRAcE	Sets the source channel of the CAN bus signal analysis or queries the current setting.	4-17
:ANALysis:SBUS<x>[:ANALyze]:I2CBus?	Queries all settings related to the I <sup>2</sup> C bus signal analysis.	4-17
:ANALysis:SBUS<x>[:ANALyze]:I2CBus:CLOCK	Sets the clock channel of the I <sup>2</sup> C bus signal analysis or queries the current setting.	4-17
:ANALysis:SBUS<x>[:ANALyze]:I2CBus:DTRace	Sets the data channel of the I <sup>2</sup> C bus signal analysis or queries the current setting.	4-17
:ANALysis:SBUS<x>[:ANALyze]:LIST?	Queries all settings related to the list display of the serial bus signal analysis.	4-17
:ANALysis:SBUS<x>[:ANALyze]:LIST:ITEM?	Queries the item in the list display of the serial bus signal analysis.	4-17
:ANALysis:SBUS<x>[:ANALyze]:LIST:MODE	Sets the mode of the list display of the serial bus signal analysis or queries the current setting.	4-17
:ANALysis:SBUS<x>[:ANALyze]:LIST:SCROll	Sets the scroll method of the list display of the serial bus signal analysis or queries the current setting.	4-18
:ANALysis:SBUS<x>[:ANALyze]:LIST:VALue?	Queries the analyzed value of the specified list display number in the serial bus signal analysis.	4-18
:ANALysis:SBUS<x>[:ANALyze]:MODE	Sets the serial bus signal analysis mode or queries the current setting.	4-18

## 4.1 A List of Commands

Command	Function	Page
ANALysis:SBUS<x>[:ANALyze]:RPOint	Sets the analysis reference point of the serial bus signal analysis or queries the current setting.	4-18
:ANALysis:SBUS<x>[:ANALyze]:SPIBus?	Queries all settings related to the SPI bus signal analysis.	4-18
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:CLOCK?	Queries all settings related to the clock channel of the SPI bus signal analysis.	4-18
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:CLOCK:POLarity	Sets the polarity of the clock channel of the SPI bus signal analysis or queries the current setting.	4-18
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:CLOCK:SOURce	Sets the clock channel of the SPI bus signal analysis or queries the current setting.	4-19
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:CS?	Queries all settings related to the chip select channel of the SPI bus signal analysis.	4-19
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:CS:ACTive	Sets the active level of the chip select channel of the SPI bus signal analysis or queries the current setting.	4-19
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:CS:TRACe	Sets the chip select channel of the SPI bus signal analysis or queries the current setting.	4-19
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:DATA<x>?	Queries all settings related to the data of the SPI bus signal analysis.	4-19
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:DATA<x>:ACTive	Sets the active level of the data of the SPI bus signal analysis or queries the current setting.	4-19
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:DATA<x>:TRACe	Sets the data channel of the SPI bus signal analysis or queries the current setting.	4-20
:ANALysis:SBUS<x>[:ANALyze]:SPIBus:SETup?	Queries all settings related to the SPI bus signal analysis setup.	4-20
:ANALysis:SBUS<x>[:ANALyze]:SPIBus[:SETup]:BITorder	Sets the bit order of the SPI bus signal analysis or queries the current setting.	4-20
:ANALysis:SBUS<x>[:ANALyze]:SPIBus[:SETup]:MODE	Sets the wiring system of the SPI bus signal analysis (three-wire or four-wire) or queries the current setting.	4-20
:ANALysis:SBUS<x>[:ANALyze]:TRACe<x>?	Queries all settings related to the threshold level of the source channel of the serial bus signal analysis.	4-20
:ANALysis:SBUS<x>[:ANALyze]:TRACe<x>:HYSTeresis	Sets the hysteresis of the threshold level of the source channel of the serial bus signal analysis or queries the current setting.	4-20
:ANALysis:SBUS<x>[:ANALyze]:TRACe<x>:LEVel	Sets the level of the threshold level of the source channel of the serial bus signal analysis or queries the current setting.	4-21
:ANALysis:SBUS<x>:ZLINKage	Sets the zoom link of the serial bus signal analysis or queries the current setting.	4-21
:ANALysis:TYPE<x>	Sets the analysis function type or queries the current setting.	4-21

## MATH Group

Command	Function	Page
:MATH<x>:OPERation	Sets the operator or queries the current setting.	4-22
:MATH<x>:SBIT?	Queries all settings related to the stuff bit computation.	4-22
:MATH<x>:SBIT:BRATe	Sets the bit rate (data transfer rate) of the stuff bit computation or queries the current setting.	4-22
:MATH<x>:SBIT:HYSTeresis	Sets the hysteresis of the stuff bit computation or queries the current setting.	4-22
:MATH<x>:SBIT:LEVel	Sets the threshold level of the stuff bit computation or queries the current setting.	4-22
:MATH<x>:SBIT:RECCessive	Sets the recessive level (bus level) of the stuff bit computation or queries the current setting.	4-22
:MATH<x>:SBIT:SPOint	Sets the sample point of the stuff bit computation or queries the current setting.	4-22

## SEARCh Group

Command	Function	Page
:SEARCh<x>:CANBus?	Queries all settings related to the CAN bus signal search.	4-23
:SEARCh<x>:CANBus:SETup?	Queries all settings related to the CAN bus signal search setup.	4-23
:SEARCh<x>:CANBus[:SETup]:ACK	Sets the ACK condition of the CAN bus signal search or queries the current setting.	4-23
:SEARCh<x>:CANBus[:SETup]:BRATe	Sets the bit rate (data transfer rate) of the CAN bus signal search or queries the current setting.	4-23
:SEARCh<x>:CANBus[:SETup]:DATA?	Queries all settings related to the CAN bus signal search data.	4-23
:SEARCh<x>:CANBus[:SETup]:DATA:BORDER	Sets the byte order of the CAN bus signal search data or queries the current setting.	4-23
:SEARCh<x>:CANBus[:SETup]:DATA:CONDition	Sets the data condition of the CAN bus signal search or queries the current setting.	4-24
:SEARCh<x>:CANBus[:SETup]:DATA:DATA<x>	Sets the comparison data of the CAN bus signal search data or queries the current setting.	4-24
:SEARCh<x>:CANBus[:SETup]:DATA:DLC	Sets the number of valid bytes (DLC) of the CAN bus signal search data or queries the current setting.	4-24
:SEARCh<x>:CANBus[:SETup]:DATA:HEXA	Sets the CAN bus signal search data in hexadecimal notation.	4-24
:SEARCh<x>:CANBus[:SETup]:DATA:MSBLsb	Sets the MSB and LSB bits of the CAN bus signal search data or queries the current setting.	4-24
:SEARCh<x>:CANBus[:SETup]:DATA:PATtern	Sets the CAN bus signal search data in binary notation or queries the current setting.	4-24
:SEARCh<x>:CANBus[:SETup]:DATA:SIGN	Sets the sign of the CAN bus signal search data or queries the current setting.	4-24
:SEARCh<x>:CANBus[:SETup]:IDEXt?	Queries all settings related to the ID of the extended format of the CAN bus signal search.	4-25
:SEARCh<x>:CANBus[:SETup]:IDEXt:HEXA	Sets the ID of the extended format of the CAN bus signal search in hexadecimal notation.	4-25
:SEARCh<x>:CANBus[:SETup]:IDEXt:PATtern	Sets the ID of the extended format of the CAN bus signal search in binary notation or queries the current setting.	4-25
:SEARCh<x>:CANBus[:SETup]:IDSTd?	Queries all settings related to the ID of the standard format of the CAN bus signal search.	4-25
:SEARCh<x>:CANBus[:SETup]:IDSTd:HEXA	Sets the ID of the standard format of the CAN bus signal search in hexadecimal notation.	4-25
:SEARCh<x>:CANBus[:SETup]:IDSTd:PATtern	Sets the ID of the standard format of the CAN bus signal search in binary notation or queries the current setting.	4-25
:SEARCh<x>:CANBus[:SETup]:MODE	Sets the CAN bus signal search mode or queries the current setting.	4-25
:SEARCh<x>:CANBus[:SETup]:RECEssive	Sets the recessive level (bus level) of the CAN bus signal search or queries the current setting.	4-25
:SEARCh<x>:CANBus[:SETup]:RTR	Sets the RTR of the CAN bus signal search or queries the current setting.	4-25
:SEARCh<x>:CANBus[:SETup]:SPoInt	Sets the sample point of the CAN bus signal search or queries the current setting.	4-26
:SEARCh<x>:CANBus[:SETup]:TRACe	Sets the source channel of the CAN bus signal search or queries the current setting.	4-26
:SEARCh<x>:I2Cbus?	Queries all settings related to the I <sup>2</sup> C bus signal search.	4-26
:SEARCh<x>:I2Cbus:CLoCK?	Queries all settings related to the clock of the I <sup>2</sup> C bus signal search.	4-26
:SEARCh<x>:I2Cbus:CLoCK:SOuRce	Sets the clock trace of the I <sup>2</sup> C bus signal search or queries the current setting.	4-26
:SEARCh<x>:I2Cbus:SETup?	Queries all settings related to the I <sup>2</sup> C bus signal search setup.	4-26
:SEARCh<x>:I2Cbus[:SETup]:ADATa?	Queries all settings related to the address of the I <sup>2</sup> C bus signal search.	4-27
:SEARCh<x>:I2Cbus[:SETup]:ADATa:BIT10address?	Queries all settings related to the 10-bit address of the I <sup>2</sup> C bus signal search.	4-27
:SEARCh<x>:I2Cbus[:SETup]:ADATa:BIT10address:HEXA	Sets the 10-bit address of the I <sup>2</sup> C bus signal search in hexadecimal notation.	4-27
:SEARCh<x>:I2Cbus[:SETup]:ADATa:BIT10address:PATtern	Sets the 10-bit address of the I <sup>2</sup> C bus signal search in binary notation or queries the current setting.	4-27

## 4.1 A List of Commands

Command	Function	Page
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7AdDress?	Queries all settings related to the 7-bit address of the I <sup>2</sup> C bus signal search.	4-27
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7AdDress:HEXA	Sets the 7-bit address of the I <sup>2</sup> C bus signal search in hexadecimal notation.	4-27
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7AdDress:PATtern	Sets the 7-bit address of the I <sup>2</sup> C bus signal search in binary notation or queries the current setting.	4-28
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7APsub?	Queries all settings related to the 7-bit + Sub address of the I <sup>2</sup> C bus signal search.	4-28
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7APsub:ADDRess?	Queries all settings related to the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal search.	4-28
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7APsub:ADDRess:HEXA	Sets the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal search in hexadecimal notation.	4-28
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7APsub:ADDRess:PATtern	Sets the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal search in binary notation or queries the current setting.	4-28
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7APsub:SADDRess?	Queries all settings related to the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal search.	4-28
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7APsub:SADDRess:HEXA	Sets the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal search in hexadecimal notation.	4-29
:SEARCH<x>:I2CBus[:SETup]:ADATa:BIT7APsub:SADDRess:PATtern	Sets the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal search in binary notation or queries the current setting.	4-29
:SEARCH<x>:I2CBus[:SETup]:ADATa:TYPE	Sets the address type of the I <sup>2</sup> C bus signal search or queries the current setting.	4-29
:SEARCH<x>:I2CBus[:SETup]:DATA?	Queries all settings related to the data of the I <sup>2</sup> C bus signal search.	4-29
:SEARCH<x>:I2CBus[:SETup]:DATA:BYTE	Sets the number of data bytes of the I <sup>2</sup> C bus signal search or queries the current setting.	4-29
:SEARCH<x>:I2CBus[:SETup]:DATA:CONDition	Sets the determination method (match or not match) of the data of the I <sup>2</sup> C bus signal search or queries the current setting.	4-29
:SEARCH<x>:I2CBus[:SETup]:DATA:DPOsition	Sets the position for comparing the data pattern of the I <sup>2</sup> C bus signal search or queries the current setting.	4-29
:SEARCH<x>:I2CBus[:SETup]:DATA:HEXA<x>	Sets the data of the I <sup>2</sup> C bus signal search in hexadecimal notation.	4-29
:SEARCH<x>:I2CBus[:SETup]:DATA:MODE	Enables/Disables the data conditions of the I <sup>2</sup> C bus signal search or queries the current setting.	4-29
:SEARCH<x>:I2CBus[:SETup]:DATA:PATtern<x>	Sets the data of the I <sup>2</sup> C bus signal search in binary notation or queries the current setting.	4-30
:SEARCH<x>:I2CBus[:SETup]:DATA:PMODE	Sets the pattern comparison start position mode of the data of the I <sup>2</sup> C bus signal search or queries the current setting.	4-30
:SEARCH<x>:I2CBus[:SETup]:GCALl?	Queries all settings related to the general call of the I <sup>2</sup> C bus signal search.	4-30
:SEARCH<x>:I2CBus[:SETup]:GCALl:BIT7maddress?	Queries all settings related to the 7-bit master address of the general call of the I <sup>2</sup> C bus signal search.	4-30
:SEARCH<x>:I2CBus[:SETup]:GCALl:BIT7maddress:HEXA	Sets the 7-bit master address of the general call of the I <sup>2</sup> C bus signal search in hexadecimal notation.	4-30
:SEARCH<x>:I2CBus[:SETup]:GCALl:BIT7maddress:PATtern	Sets the 7-bit master address of the general call of the I <sup>2</sup> C bus signal search in binary notation or queries the current setting.	4-30

Command	Function	Page
:SEARCH<x>:I2CBus[:SETup]:GCALl:SBYTe	Sets the second byte type of the general call of the I <sup>2</sup> C bus signal search or queries the current setting.	4-30
:SEARCH<x>:I2CBus[:SETup]:MODE	Sets the search mode of the I <sup>2</sup> C bus signal search or queries the current setting.	4-31
:SEARCH<x>:I2CBus[:SETup]:NAIGnore?	Queries all settings related to the NON ACK ignore mode of the I <sup>2</sup> C bus signal search.	4-31
:SEARCH<x>:I2CBus[:SETup]:NAIGnore:HSMoDe	Sets whether to ignore NON ACK in high speed mode of the I <sup>2</sup> C bus signal search or queries the current setting.	4-31
:SEARCH<x>:I2CBus[:SETup]:NAIGnore:RACcEss	Sets whether to ignore NON ACK in read access mode of the I <sup>2</sup> C bus signal search or queries the current setting.	4-31
:SEARCH<x>:I2CBus[:SETup]:NAIGnore:SBYTe	Sets whether to ignore NON ACK in the start byte of the I <sup>2</sup> C bus signal search or queries the current setting.	4-31
:SEARCH<x>:I2CBus[:SETup]:SBHSmode?	Queries all settings related to the start byte and high speed mode of the I <sup>2</sup> C bus signal search.	4-31
:SEARCH<x>:I2CBus[:SETup]:SBHSmode:TYPe	Sets the type of the start byte or high speed mode of the I <sup>2</sup> C bus signal search or queries the current setting.	4-31
:SEARCH<x>:SPIBus?	Queries all settings related to the SPI bus signal search.	4-32
:SEARCH<x>:SPIBus:CLOCK	Queries all settings related to the clock channel of the SPI bus signal search.	4-32
:SEARCH<x>:SPIBus:CLOCK:POLarity	Sets the polarity of the clock channel of the SPI bus signal search or queries the current setting.	4-32
:SEARCH<x>:SPIBus:CLOCK:SOURce	Sets the clock channel of the SPI bus signal search or queries the current setting.	4-32
:SEARCH<x>:SPIBus:CS?	Queries all settings related to the chip select channel of the SPI bus signal search.	4-32
:SEARCH<x>:SPIBus:CS:ACTive	Sets the active level of the chip select channel of the SPI bus signal search or queries the current setting.	4-32
:SEARCH<x>:SPIBus:CS:TRACe	Sets the chip select channel of the SPI bus signal search or queries the current setting.	4-32
:SEARCH<x>:SPIBus:SETup?	Queries all settings related to the SPI bus signal search setup.	4-32
:SEARCH<x>:SPIBus[:SETup]:BITorder	Sets the bit order of the SPI bus signal search or queries the current setting.	4-33
:SEARCH<x>:SPIBus[:SETup]:DATA<x>?	Queries all settings related to the data of the SPI bus signal search.	4-33
:SEARCH<x>:SPIBus[:SETup]:DATA<x>:BYTe	Sets the number of bytes of the data of the SPI bus signal search or queries the current setting.	4-33
:SEARCH<x>:SPIBus[:SETup]:DATA<x>:CONDition	Sets the determination method (match or not match) of the data of the SPI bus signal search or queries the current setting.	4-33
:SEARCH<x>:SPIBus[:SETup]:DATA<x>:DPOsition	Sets the pattern comparison start position of the data of the SPI bus signal search or queries the current setting.	4-33
:SEARCH<x>:SPIBus[:SETup]:DATA<x>:HEXA<x>	Sets the data of the SPI bus signal search in hexadecimal notation.	4-33
:SEARCH<x>:SPIBus[:SETup]:DATA<x>:PATTeRn<x>	Sets the data of the SPI bus signal search in binary notation or queries the current setting.	4-33
:SEARCH<x>:SPIBus[:SETup]:DATA<x>:TRACe	Sets the source channel of the data of the SPI bus signal search or queries the current setting.	4-33
:SEARCH<x>:SPIBus[:SETup]:MODE	Sets the wiring system of the SPI bus signal search (three-wire or four-wire) or queries the current setting.	4-34
:SEARCH<x>:STRace	Sets the search source channel or queries the current setting.	4-34
:SEARCH<x>:TRACe<x>:LEVeL	Sets the threshold level of the trace or queries the current setting.	4-34
:SEARCH<x>:TYPe	Sets the search type or queries the current setting.	4-34

## 4.1 A List of Commands

### TRIGger Group

Command	Function	Page
:TRIGger:EINterval:EVENT<x>:CANBus?	Queries all settings related to the CAN bus trigger of the event.	4-35
:TRIGger:EINterval:EVENT<x>:CANBus:ACK	Sets the ACK condition of the CAN bus signal trigger or queries the current setting.	4-35
:TRIGger:EINterval:EVENT<x>:CANBus:BRATe	Sets the bit rate (data transfer rate) of the CAN bus signal trigger or queries the current setting.	4-35
:TRIGger:EINterval:EVENT<x>:CANBus:DATA?	Queries all settings related to the CAN bus signal trigger data.	4-35
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:BORDer	Sets the byte order of the CAN bus signal trigger data or queries the current setting.	4-36
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:CONDition	Sets the data condition of the CAN bus signal trigger or queries the current setting.	4-36
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:DATA<x>	Sets the comparison data of the CAN bus signal trigger data or queries the current setting.	4-36
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:DLC	Sets the number of valid bytes (DLC) of the CAN bus signal trigger data or queries the current setting.	4-36
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:HEXA	Sets the CAN bus signal trigger data in hexadecimal notation.	4-37
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:MSBLsb	Sets the MSB and LSB bits of the CAN bus signal trigger data or queries the current setting.	4-37
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:PATtern	Sets the CAN bus signal trigger data in binary notation or queries the current setting.	4-37
:TRIGger:EINterval:EVENT<x>:CANBus:DATA:SIGN	Sets the sign of the CAN bus signal trigger data or queries the current setting.	4-37
:TRIGger:EINterval:EVENT<x>:CANBus:IDExt?	Queries all settings related to the ID of the extended format of the CAN bus signal trigger.	4-37
:TRIGger:EINterval:EVENT<x>:CANBus:IDExt:HEXA	Sets the ID of the extended format of the CAN bus signal trigger in hexadecimal notation.	4-37
:TRIGger:EINterval:EVENT<x>:CANBus:IDExt:PATtern	Sets the ID of the extended format of the CAN bus signal trigger in binary notation or queries the current setting.	4-38
:TRIGger:EINterval:EVENT<x>:CANBus:IDOR?	Queries all settings related to the OR condition of the CAN bus signal trigger.	4-38
:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>?	Queries all settings related to each ID of the OR condition of the CAN bus signal trigger.	4-38
:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:ACK	Sets each ACK condition of the OR condition of the CAN bus signal trigger or queries the current setting.	4-38
:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA?	Queries all settings related to each data of the OR condition of the CAN bus signal trigger.	4-39
:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:BORDer	Sets byte order of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-39
:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:CONDition	Sets each data condition of the OR condition of the CAN bus signal trigger or queries the current setting.	4-39



Command	Function	Page
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:DATA<x>	Sets comparison data of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-39
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:DLC	Sets the number of valid bytes (DLC) of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-39
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:HEXA	Sets each data of the OR condition of the CAN bus signal trigger in hexadecimal notation.	4-40
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:MSBLSb	Sets the MSB and LSB bits of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-40
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:PATtern	Sets each data of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.	4-40
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:SIGN	Sets sign of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-40
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:FORMat	Sets each message format (standard or extended) of the OR condition of the CAN bus signal trigger or queries the current setting.	4-40
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:IDEXt?	Queries all settings related to the ID of each extended format of the OR condition of the CAN bus signal trigger.	4-40
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:IDEXt:HEXA	Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in hexadecimal notation.	4-41
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:IDEXt:PATtern	Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.	4-41
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:IDSTd?	Queries all settings related to the ID of each standard format of the OR condition of the CAN bus signal trigger.	4-41
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:IDSTd:HEXA	Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in hexadecimal notation.	4-41
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:IDSTd:PATtern	Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.	4-41
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:MODE	Enables or disables each condition of the OR condition of the CAN bus signal trigger or queries the current setting.	4-41
:TRIGger:EINTerval:EVENT<x>:CANBus:IDOR:ID<x>:RTR	Sets each RTR of the OR condition of the CAN bus signal trigger or queries the current setting.	4-41
:TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd?	Queries all settings related to the ID of the standard format of the CAN bus signal trigger.	4-42
:TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd:HEXA	Sets the ID of the standard format of the CAN bus signal trigger in hexadecimal notation.	4-42
:TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd:PATtern	Sets the ID of the standard format of the CAN bus signal trigger in binary notation or queries the current setting.	4-42
:TRIGger:EINTerval:EVENT<x>:CANBus:MODE	Sets the CAN bus signal trigger mode or queries the current setting.	4-42

## 4.1 A List of Commands

Command	Function	Page
:TRIGger:EINterval:EVENT<x>:CANBus:RECEssive	Sets the recessive level (bus level) of the CAN bus signal trigger or queries the current setting.	4-42
:TRIGger:EINterval:EVENT<x>:CANBus:RTR	Sets the RTR of the CAN bus signal trigger or queries the current setting.	4-42
:TRIGger:EINterval:EVENT<x>:CANBus:SOURce	Sets the trigger source of the CAN bus signal trigger or queries the current setting.	4-42
:TRIGger:EINterval:EVENT<x>:CANBus:SPOint	Sets the sample point of the CAN bus signal trigger or queries the current setting.	4-43
:TRIGger:EINterval:EVENT<x>:I2CBus?	Queries all settings related to the I <sup>2</sup> C bus signal trigger of the event.	4-24
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa?	Queries all settings related to the address of the I <sup>2</sup> C bus signal trigger.	4-43
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT10address?	Queries all settings related to the 10-bit address of the I <sup>2</sup> C bus signal trigger.	4-43
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT10address:HEXA	Sets the 10-bit address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-43
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT10address:PATtern	Sets the 10-bit address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-44
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7Address?	Queries all settings related to the 7-bit address of the I <sup>2</sup> C bus signal trigger.	4-44
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7Address:HEXA	Sets the 7-bit address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-44
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7Address:PATtern	Sets the 7-bit address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-44
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7APsub?	Queries all settings related to the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger.	4-44
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7APsub:ADDRess?	Queries all settings related to the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger.	4-44
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7APsub:ADDRess:HEXA	Sets the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-45
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7APsub:ADDRess:PATtern	Sets the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-45
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7APsub:SADDRess?	Queries all settings related to the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger.	4-45
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7APsub:SADDRess:HEXA	Sets the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-45
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:BIT7APsub:SADDRess:PATtern	Sets the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-45
:TRIGger:EINterval:EVENT<x>:I2CBus:ADATa:TYPE	Sets the address type of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-45
:TRIGger:EINterval:EVENT<x>:I2CBus:CLOCK?	Queries all settings related to the clock channel of the I <sup>2</sup> C bus signal trigger.	4-45
:TRIGger:EINterval:EVENT<x>:I2CBus:CLOCK:SOURce	Sets the clock channel of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-46
:TRIGger:EINterval:EVENT<x>:I2CBus:DATA?	Queries all settings related to the data of the I <sup>2</sup> C bus signal trigger.	4-46

Command	Function	Page
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:BYTE	Sets the number of data bytes of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-46
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:CONDition	Sets the determination method (match or not matched) of the data of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-46
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:DPOsition	Sets the position for comparing the data pattern of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-46
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:HEXA<x>	Sets the data of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-46
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:MODE	Enables/Disables the data conditions of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-47
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:PATtern<x>	Sets the data of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-47
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:PMODE	Sets the pattern comparison start position mode of the data of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-47
:TRIGger:EINTerval:EVENT<x>:I2CBus:DATA:SOURce	Sets the data channel of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-47
:TRIGger:EINTerval:EVENT<x>:I2CBus:GCALL?	Queries all settings related to the general call of the I <sup>2</sup> C bus signal trigger.	4-47
:TRIGger:EINTerval:EVENT<x>:I2CBus:GCALL:BIT7maddress?	Queries all settings related to the 7-bit master address of the general call of the I <sup>2</sup> C bus signal trigger.	4-47
:TRIGger:EINTerval:EVENT<x>:I2CBus:GCALL:BIT7maddress:HEXA	Sets the 7-bit master address of the general call of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-47
:TRIGger:EINTerval:EVENT<x>:I2CBus:GCALL:BIT7maddress:PATtern	Sets the 7-bit master address of the general call of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-48
:TRIGger:EINTerval:EVENT<x>:I2CBus:GCALL:SBYTE	Sets the second byte type of the general call of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-48
:TRIGger:EINTerval:EVENT<x>:I2CBus:MODE	Sets the trigger mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-48
:TRIGger:EINTerval:EVENT<x>:I2CBus:NAIGnore?	Queries all settings related to the NON ACK ignore mode of the I <sup>2</sup> C bus signal trigger.	4-48
:TRIGger:EINTerval:EVENT<x>:I2CBus:NAIGnore:HSMODE	Sets whether to ignore NON ACK in high speed mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-48
:TRIGger:EINTerval:EVENT<x>:I2CBus:NAIGnore:RACcESS	Sets whether to ignore NON ACK in read access mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-48
:TRIGger:EINTerval:EVENT<x>:I2CBus:NAIGnore:SBYTE	Sets whether to ignore NON ACK in the start byte of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-49
:TRIGger:EINTerval:EVENT<x>:I2CBus:SBHSMODE?	Queries all settings related to the start byte and high speed mode of the I <sup>2</sup> C bus signal trigger.	4-49
:TRIGger:EINTerval:EVENT<x>:I2CBus:SBHSMODE:TYPE	Sets the type of the start byte or high speed mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-49
:TRIGger:EINTerval:EVENT<x>:SPIBus?	Queries all settings related to the SPI bus signal trigger of the event.	4-49

## 4.1 A List of Commands

Command	Function	Page
:TRIGger:EINterval:EVENT<x>:SPIBus:BITorder	Sets the bit order of the SPI bus signal trigger or queries the current setting.	4-49
:TRIGger:EINterval:EVENT<x>:SPIBus:CLOCK?	Queries all settings related to the clock channel of the SPI bus signal trigger.	4-49
:TRIGger:EINterval:EVENT<x>:SPIBus:CLOCK:POLarity	Sets the polarity of the clock channel of the SPI bus signal trigger or queries the current setting.	4-50
:TRIGger:EINterval:EVENT<x>:SPIBus:CLOCK:SOURce	Sets the clock channel of the SPI bus signal trigger or queries the current setting.	4-50
:TRIGger:EINterval:EVENT<x>:SPIBus:CS?	Queries all settings related to the chip select channel of the SPI bus signal trigger.	4-50
:TRIGger:EINterval:EVENT<x>:SPIBus:CS:ACTive	Sets the active level of the chip select channel of the SPI bus signal trigger or queries the current setting.	4-50
:TRIGger:EINterval:EVENT<x>:SPIBus:CS:SOURce	Sets the chip select channel of the SPI bus signal trigger or queries the current setting.	4-50
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>?	Queries all settings related to the data of the SPI bus signal trigger.	4-50
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:BYTE	Sets the number of bytes of the data of the SPI bus signal trigger or queries the current setting.	4-51
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:CONDition	Sets the determination method (match or not match) of the data of the SPI bus signal trigger or queries the current setting.	4-51
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:DPOSition	Sets the pattern comparison start position of the data of the SPI bus trigger or queries the current setting.	4-51
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:HEXA<x>	Sets the data of the SPI bus signal trigger in hexadecimal notation.	4-51
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:PATtern<x>	Sets the data of the SPI bus signal trigger in binary notation or queries the current setting.	4-51
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:SOURce	Sets the trace of the data of the SPI bus signal trigger or queries the current setting.	4-51
:TRIGger:EINterval:EVENT<x>:SPIBus:MODE	Sets the wiring system of the SPI bus signal trigger (three-wire or four-wire) or queries the current setting.	4-52
:TRIGger:EINterval:EVENT<x>:STATE:CHANnel<x>	Sets the condition to be satisfied of the channel or queries the current setting.	4-52
:TRIGger:EINterval:EVENT<x>:TYPE	Sets the trigger type of the event or queries the current setting.	4-52
:TRIGger:ENHanced:CANBus?	Queries all settings related to the CAN bus signal trigger.	4-52
:TRIGger:ENHanced:CANBus:ACK	Sets the ACK condition of the CAN bus signal trigger or queries the current setting.	4-52
:TRIGger:ENHanced:CANBus:BRATe	Sets the bit rate (data transfer rate) of the CAN bus signal trigger or queries the current setting.	4-53
:TRIGger:ENHanced:CANBus:DATA?	Queries all settings related to the CAN bus signal trigger data.	4-53
:TRIGger:ENHanced:CANBus:DATA:BORDer	Sets the byte order of the CAN bus signal trigger data or queries the current setting.	4-53
:TRIGger:ENHanced:CANBus:DATA:CONDition	Sets the data condition of the CAN bus signal trigger or queries the current setting.	4-53
:TRIGger:ENHanced:CANBus:DATA:DATA<x>	Sets the comparison data of the CAN bus signal trigger data or queries the current setting.	4-53

Command	Function	Page
:TRIGger:ENHanced:CANBus:DATA:DLC	Sets the number of valid bytes (DLC) of the CAN bus signal trigger data or queries the current setting.	4-53
:TRIGger:ENHanced:CANBus:DATA:HEXA	Sets the CAN bus signal trigger data in hexadecimal notation.	4-53
:TRIGger:ENHanced:CANBus:DATA:MSBLsb	Sets the MSB and LSB bits of the CAN bus signal trigger data or queries the current setting.	4-54
:TRIGger:ENHanced:CANBus:DATA:PATtern	Sets the CAN bus signal trigger data in binary notation or queries the current setting.	4-54
:TRIGger:ENHanced:CANBus:DATA:SIGN	Sets the sign of the CAN bus signal trigger data or queries the current setting.	4-54
:TRIGger:ENHanced:CANBus:IDExt?	Queries all settings related to the ID of the extended format of the CAN bus signal trigger.	4-54
:TRIGger:ENHanced:CANBus:IDExt:HEXA	Sets the ID of the extended format of the CAN bus signal trigger in hexadecimal notation.	4-54
:TRIGger:ENHanced:CANBus:IDExt:PATtern	Sets the ID of the extended format of the CAN bus signal trigger in binary notation or queries the current setting.	4-54
:TRIGger:ENHanced:CANBus:IDOR?	Queries all settings related to the OR condition of the CAN bus signal trigger.	4-54
:TRIGger:ENHanced:CANBus:IDOR:ID<x>?	Queries all settings related to each ID of the OR condition of the CAN bus signal trigger.	4-55
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:ACK	Sets each ACK condition of the OR condition of the CAN bus signal trigger or queries the current setting.	4-55
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA?	Queries all settings related to each data of the OR condition of the CAN bus signal trigger.	4-55
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:BORder	Sets byte order of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-55
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:CONDition	Sets each data condition of the OR condition of the CAN bus signal trigger or queries the current setting.	4-55
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:DATA<x>	Sets comparison data of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-56
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:DLC	Sets the number of valid bytes (DLC) of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-56
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:HEXA	Sets each data of the OR condition of the CAN bus signal trigger in hexadecimal notation.	4-56
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:MSBLsb	Sets the MSB and LSB bits of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-56
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:PATtern	Sets each data of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.	4-56
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:SIGN	Sets sign of each data of the OR condition of the CAN bus signal trigger or queries the current setting.	4-57
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:FORMat	Sets each message format (standard or extended) of the OR condition of the CAN bus signal trigger or queries the current setting.	4-57

## 4.1 A List of Commands

Command	Function	Page
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:IDEXt?	Queries all settings related to the ID of each extended format of the OR condition of the CAN bus signal trigger.	4-57
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:IDEXt:HEXA	Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in hexadecimal notation.	4-57
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:IDEXt:PATtern	Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.	4-57
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:IDSTd?	Queries all settings related to the ID of each standard format of the OR condition of the CAN bus signal trigger.	4-57
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:IDSTd:HEXA	Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in hexadecimal notation.	4-57
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:IDSTd:PATtern	Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.	4-58
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:MODE	Enables or disables each condition of the OR condition of the CAN bus signal trigger or queries the current setting.	4-58
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:RTR	Sets each RTR of the OR condition of the CAN bus signal trigger or queries the current setting.	4-58
:TRIGger:ENHanced:CANBus:IDSTd?	Queries all settings related to the ID of the standard format of the CAN bus signal trigger.	4-58
:TRIGger:ENHanced:CANBus:IDSTd:HEXA	Sets the ID of the standard format of the CAN bus signal trigger in hexadecimal notation.	4-58
:TRIGger:ENHanced:CANBus:IDSTd:PATtern	Sets the ID of the standard format of the CAN bus signal trigger in binary notation or queries the current setting.	4-58
:TRIGger:ENHanced:CANBus:MODE	Sets the CAN bus signal trigger mode or queries the current setting.	4-58
:TRIGger:ENHanced:CANBus:REcessive	Sets the recessive level (bus level) of the CAN bus signal trigger or queries the current setting.	4-58
:TRIGger:ENHanced:CANBus:RTR	Sets the RTR of the CAN bus signal trigger or queries the current setting.	4-59
:TRIGger:ENHanced:CANBus:SOURce	Sets the trigger source of the CAN bus signal trigger or queries the current setting.	4-59
:TRIGger:ENHanced:CANBus:SPOint	Sets the sample point of the CAN bus signal trigger or queries the current setting.	4-59
:TRIGger:ENHanced:I2CBus?	Queries all settings related to the I <sup>2</sup> C bus signal trigger.	4-59
:TRIGger:ENHanced:I2CBus:ADATa?	Queries all settings related to the address of the I <sup>2</sup> C bus signal trigger.	4-59
:TRIGger:ENHanced:I2CBus:ADATa:BIT10address?	Queries all settings related to the 10-bit address of the I <sup>2</sup> C bus signal trigger.	4-59
:TRIGger:ENHanced:I2CBus:ADATa:BIT10address:HEXA	Sets the 10-bit address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-60
:TRIGger:ENHanced:I2CBus:ADATa:BIT10address:PATtern	Sets the 10-bit address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-60
:TRIGger:ENHanced:I2CBus:ADATa:BIT7Address?	Queries all settings related to the 7-bit address of the I <sup>2</sup> C bus signal trigger.	4-60
:TRIGger:ENHanced:I2CBus:ADATa:BIT7Address:HEXA	Sets the 7-bit address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-60
:TRIGger:ENHanced:I2CBus:ADATa:BIT7Address:PATtern	Sets the 7-bit address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-60

Command	Function	Page
:TRIGger:ENHanced:I2CBus:ADATa:BIT7APsub?	Queries all settings related to the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger.	4-60
:TRIGger:ENHanced:I2CBus:ADATa:BIT7APsub:ADDRESS?	Queries all settings related to the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger.	4-60
:TRIGger:ENHanced:I2CBus:ADATa:BIT7APsub:ADDRESS:HEXA	Sets the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-60
:TRIGger:ENHanced:I2CBus:ADATa:BIT7APsub:ADDRESS:PATtern	Sets the 7-bit address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-61
:TRIGger:ENHanced:I2CBus:ADATa:BIT7APsub:SADDRESS?	Queries all settings related to the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger.	4-61
:TRIGger:ENHanced:I2CBus:ADATa:BIT7APsub:SADDRESS:HEXA	Sets the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-61
:TRIGger:ENHanced:I2CBus:ADATa:BIT7APsub:SADDRESS:PATtern	Sets the Sub address of the 7-bit + Sub address of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-61
:TRIGger:ENHanced:I2CBus:ADATa:TYPE	Sets the address type of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-61
:TRIGger:ENHanced:I2CBus:CLOCK?	Queries all settings related to the clock channel of the I <sup>2</sup> C bus signal trigger.	4-61
:TRIGger:ENHanced:I2CBus:CLOCK:SOURce	Sets the clock channel of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-61
:TRIGger:ENHanced:I2CBus:DATA?	Queries all settings related to the data of the I <sup>2</sup> C bus signal trigger.	4-61
:TRIGger:ENHanced:I2CBus:DATA:BYTE	Sets the number of data bytes of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-62
:TRIGger:ENHanced:I2CBus:DATA:CONDition	Sets the determination method (match or not matched) of the data of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-62
:TRIGger:ENHanced:I2CBus:DATA:DPOSITion	Sets the position for comparing the data pattern of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-62
:TRIGger:ENHanced:I2CBus:DATA:HEXA<x>	Sets the data of the I <sup>2</sup> C bus signal trigger in hexadecimal notation.	4-62
:TRIGger:ENHanced:I2CBus:DATA:MODE	Enables/Disables the data conditions of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-62
:TRIGger:ENHanced:I2CBus:DATA:PATtern<x>	Sets the data of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-62
:TRIGger:ENHanced:I2CBus:DATA:PMODE	Sets the pattern comparison start position mode of the data of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-62
:TRIGger:ENHanced:I2CBus:DATA:SOURce	Sets the data channel of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-62
:TRIGger:ENHanced:I2CBus:GCALL?	Queries all settings related to the general call of the I <sup>2</sup> C bus signal trigger.	4-63
:TRIGger:ENHanced:I2CBus:GCALL:BIT7maddress?	Queries all settings related to the 7-bit master address of the general call of the I <sup>2</sup> C bus signal trigger.	4-63
:TRIGger:ENHanced:I2CBus:GCALL:BIT7maddress:HEXA	Sets the 7-bit master address of the general call of the I <sup>2</sup> C bus trigger in hexadecimal notation.	4-63
:TRIGger:ENHanced:I2CBus:GCALL:BIT7maddress:PATtern	Sets the 7-bit master address of the general call of the I <sup>2</sup> C bus signal trigger in binary notation or queries the current setting.	4-63
:TRIGger:ENHanced:I2CBus:GCALL:SBYTE	Sets the second byte type of the general call of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-63
:TRIGger:ENHanced:I2CBus:MODE	Sets the trigger mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-63

## 4.1 A List of Commands

Command	Function	Page
:TRIGger:ENHanced:I2CBus:NAIgnore?	Queries all settings related to the NON ACK ignore mode of the I <sup>2</sup> C bus signal trigger.	4-63
:TRIGger:ENHanced:I2CBus:NAIgnore:HSMoDe	Sets whether to ignore NON ACK in high speed mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-63
:TRIGger:ENHanced:I2CBus:NAIgnore:RACcEss	Sets whether to ignore NON ACK in read access mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-64
:TRIGger:ENHanced:I2CBus:NAIgnore:SBYTe	Sets whether to ignore NON ACK in the start byte of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-64
:TRIGger:ENHanced:I2CBus:SBHSMoDe?	Queries all settings related to the start byte and high speed mode of the I <sup>2</sup> C bus signal trigger.	4-64
:TRIGger:ENHanced:I2CBus:SBHSMoDe:TYPe	Sets the type of the start byte or high speed mode of the I <sup>2</sup> C bus signal trigger or queries the current setting.	4-64
:TRIGger:ENHanced:SPIBus?	Queries all settings related to the SPI bus signal trigger.	4-64
:TRIGger:ENHanced:SPIBus:BIToRder	Sets the bit order of the SPI bus signal trigger or queries the current setting.	4-64
:TRIGger:ENHanced:SPIBus:ClOck?	Queries all settings related to the clock channel of the SPI bus signal trigger.	4-64
:TRIGger:ENHanced:SPIBus:ClOck:POLarity	Sets the polarity of the clock channel of the SPI bus signal trigger or queries the current setting.	4-64
:TRIGger:ENHanced:SPIBus:ClOck:SOURce	Sets the clock channel of the SPI bus signal trigger or queries the current setting.	4-65
:TRIGger:ENHanced:SPIBus:CS?	Queries all settings related to the chip select channel of the SPI bus signal trigger.	4-65
:TRIGger:ENHanced:SPIBus:CS:ACTive	Sets the active level of the chip select channel of the SPI bus signal trigger or queries the current setting.	4-65
:TRIGger:ENHanced:SPIBus:CS:SOURce	Sets the chip select channel of the SPI bus signal trigger or queries the current setting.	4-65
:TRIGger:ENHanced:SPIBus:DATA<x>?	Queries all settings related to the data of the SPI bus signal trigger.	4-65
:TRIGger:ENHanced:SPIBus:DATA<x>:BYTe	Sets the number of bytes of the data of the SPI bus signal trigger or queries the current setting.	4-65
:TRIGger:ENHanced:SPIBus:DATA<x>:CONDition	Sets the determination method (match or not match) of the data of the SPI bus signal trigger or queries the current setting.	4-65
:TRIGger:ENHanced:SPIBus:DATA<x>:DPOsition	Sets the pattern comparison start position of the data of the SPI bus signal trigger or queries the current setting.	4-65
:TRIGger:ENHanced:SPIBus:DATA<x>:HEXA<x>	Sets the data of the SPI bus signal trigger in hexadecimal notation.	4-66
:TRIGger:ENHanced:SPIBus:DATA<x>:PATTeRn<x>	Sets the data of the SPI bus signal trigger in binary notation or queries the current setting.	4-66
:TRIGger:ENHanced:SPIBus:DATA<x>:SOURce	Sets the source channel of the data of the SPI bus signal trigger or queries the current setting.	4-66
:TRIGger:ENHanced:SPIBus::MODE	Sets the wiring system of the SPI bus signal trigger (three-wire or four-wire) or queries the current setting.	4-66
:TRIGger:SOURce:CHANnel<x>:LEVEl	Sets the trigger level of the channel or queries the current setting.	4-66
:TRIGger:SOURce:CHANnel<x>:STATe	Sets the condition to be satisfied of the channel or queries the current setting.	4-66
:TRIGger:TYPe	Sets the trigger type or queries the current setting.	4-66



## 4.2 ANALysis Group

### **:ANALysis:SBUS<x>?**

**Function** Queries all settings related to the serial bus signal analysis function.

**Syntax** :ANALysis:SBUS<x>?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1? ->  
:ANALYSIS:SBUS1:ANALYZE:CANBUS:  
BRATE 1000000;RECESSIVE HIGH;  
SPOINT 62.5E+00;TRACE 1;:ANALYSIS:  
SBUS1:ANALYZE:I2CBUS:CLOCK 1;DTRACE 1;:  
ANALYSIS:SBUS1:ANALYZE:LIST:  
MODE DETAIL;SCROLL HORIZONTAL;:  
ANALYSIS:SBUS1:ANALYZE:MODE CANBUS;  
MPOSITION 0.00000E+00;  
RPOINTTRIGGER;SPIBUS:CLOCK:  
POLARITY FALL;SOURCE 1;:ANALYSIS:SBUS1:  
ANALYZE:SPIBUS:CS:ACTIVE HIGH;TRACE 1;:  
ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:  
ACTIVE HIGH;TRACE 1;:ANALYSIS:SBUS1:  
ANALYZE:SPIBUS:DATA2:ACTIVE HIGH;  
TRACE 1;:ANALYSIS:SBUS1:ANALYZE:SPIBUS:  
SETUP:BITORDER LSBFIRST;MODE WIRE3;:  
ANALYSIS:SBUS1:ANALYZE:TRACE1:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE2:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE3:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE4:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE5:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE6:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE7:  
HYSTERESIS 1.000E+00;LEVEL  
1.000E+00;:ANALYSIS:SBUS1:ANALYZE:  
TRACE8:HYSTERESIS 1.000E+00;  
LEVEL 1.000E+00;:ANALYSIS:SBUS1:  
ZLINKAGE OFF

### **:ANALysis:SBUS<x>:ANALyze?**

**Function** Queries all settings related to the serial bus signal analysis.

**Syntax** :ANALysis:SBUS<x>:ANALyze?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1:ANALYZE? ->  
:ANALYSIS:SBUS1:ANALYZE:CANBUS:  
BRATE 1000000;RECESSIVE HIGH;  
SPOINT 62.5E+00;TRACE 1;:ANALYSIS:  
SBUS1:ANALYZE:I2CBUS:CLOCK 1;DTRACE 1;:  
ANALYSIS:SBUS1:ANALYZE:LIST:  
MODE DETAIL;SCROLL HORIZONTAL;:  
ANALYSIS:SBUS1:ANALYZE:MODE CANBUS;  
MPOSITION 0.00000E+00;RPOINT TRIGGER;  
SPIBUS:CLOCK:POLARITY FALL;SOURCE 1;:  
ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:  
ACTIVE HIGH;TRACE 1;:ANALYSIS:SBUS1:  
ANALYZE:SPIBUS:DATA1:ACTIVE HIGH;  
TRACE 1;:ANALYSIS:SBUS1:ANALYZE:SPIBUS:  
DATA2:ACTIVE HIGH;TRACE 1;:ANALYSIS:  
SBUS1:ANALYZE:SPIBUS:SETUP:  
BITORDER LSBFIRST;MODE WIRE3;:ANALYSIS:  
SBUS1:ANALYZE:TRACE1:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE2:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE3:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE4:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE5:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE6:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE7:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00;:  
ANALYSIS:SBUS1:ANALYZE:TRACE8:  
HYSTERESIS 1.000E+00;LEVEL 1.000E+00

### **:ANALysis:SBUS<x>[:ANALyze]:CANBus?**

**Function** Queries all settings related to the CAN bus signal analysis.

**Syntax** :ANALysis:SBUS<x>[:ANALyze]:CANBus?  
<x> = 1, 2

**Example** :ANALYSIS:SBUS1:ANALYZE:CANBUS? ->  
:ANALYSIS:SBUS1:ANALYZE:CANBUS:  
BRATE 1000000;RECESSIVE HIGH;  
SPOINT 62.5E+00;TRACE 1

## 4.2 ANALYSIS Group

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **BRATE**

Function Sets the bit rate (data transfer rate) of the CAN bus signal analysis or queries the current setting.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**BRATE {<Nrf>|USER,<Nrf>}**

**:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**BRATE?**

**<x> = 1, 2**

**<Nrf> = 83300, 125000, 250000, 500000, 1000000**

signal **<Nrf> of USER = See the *User's Manual (IM701310-01E)*.**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:**

**BRATE 83300**

**:ANALYSIS:SBUS1:ANALYZE:CANBUS:**

**BRATE? ->**

**:ANALYSIS:SBUS1:ANALYZE:CANBUS:**

**BRATE 83300**

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **FJUMP:ACK**

Function Executes a field jump to the ACK Field in the results of the CAN bus signal analysis.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**FJUMP:ACK**

**<x> = 1, 2**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:FJUMP:**

**ACK**

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **FJUMP:CONTROL**

Function Executes a field jump to the Control Field in the results of the CAN bus signal analysis.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**FJUMP:CONTROL**

**<x> = 1, 2**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:FJUMP:**

**CONTROL**

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **FJUMP:CRC**

Function Executes a field jump to the CRC Field in the results of the CAN bus signal analysis.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**FJUMP:CRC**

**<x> = 1, 2**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:FJUMP:**

**CRC**

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **FJUMP:DATA**

Function Executes a field jump to the Data Field in the results of the CAN bus signal analysis.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**FJUMP:DATA**

**<x> = 1, 2**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:FJUMP:**

**DATA**

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **FJUMP:IDENTIFIER**

Function Executes a field jump to the Identifier Field in the results of the CAN bus signal analysis.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**FJUMP:IDENTIFIER**

**<x> = 1, 2**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:FJUMP:**

**IDENTIFIER**

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **FJUMP:SOF**

Function Executes a field jump to the SOF Field in the results of the CAN bus signal analysis.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**FJUMP:SOF**

**<x> = 1, 2**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:FJUMP:**

**SOF**

### **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

#### **RECESSIVE**

Function Sets the recessive level (bus level) of the CAN bus signal analysis or queries the current setting.

Syntax **:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**RECESSIVE {HIGH|LOW}**

**:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:**

**RECESSIVE?**

**<x> = 1, 2**

Example **:ANALYSIS:SBUS1:ANALYZE:CANBUS:**

**RECESSIVE HIGH**

**:ANALYSIS:SBUS1:ANALYZE:CANBUS:**

**RECESSIVE? ->**

**:ANALYSIS:SBUS1:ANALYZE:CANBUS:**

**RECESSIVE HIGH**

**:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:****SPOINT**

Function Sets the sample point of the CAN bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:  
SPOINT {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:  
SPOINT?  
<x> = 1, 2  
<NRf> = 18.8 to 90.6(%)

Example :ANALYSIS:SBUS1:ANALYZE:CANBUS:  
SPOINT 18.8  
:ANALYSIS:SBUS1:ANALYZE:CANBUS:  
SPOINT? ->  
:ANALYSIS:SBUS1:ANALYZE:CANBUS:  
SPOINT 18.8E+00

**:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:****TRACE**

Function Sets the trace of the CAN bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:  
TRACE {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:CANBUS:  
TRACE?  
<x> = 1, 2  
<NRf> = 1 to 8

Example :ANALYSIS:SBUS1:ANALYZE:CANBUS:TRACE 1  
:ANALYSIS:SBUS1:ANALYZE:CANBUS:  
TRACE? ->  
:ANALYSIS:SBUS1:ANALYZE:CANBUS:TRACE 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS?**

Function Queries all settings related to the I<sup>2</sup>C bus signal analysis.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:I2CBUS? ->  
:ANALYSIS:SBUS1:ANALYZE:I2CBUS:CLOCK 1;  
DTRACE 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS:****CLOCK**

Function Sets the clock channel of the I<sup>2</sup>C bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS:  
CLOCK {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS:  
CLOCK?  
<x> = 1 or 2  
<NRf> = 1 to 8

Example :ANALYSIS:SBUS1:ANALYZE:I2CBUS:CLOCK 1  
:ANALYSIS:SBUS1:ANALYZE:I2CBUS:CLOCK? ->  
:ANALYSIS:SBUS1:ANALYZE:I2CBUS:  
CLOCK 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS:****DTRACE**

Function Sets the data channel of the I<sup>2</sup>C bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS:  
DTRACE {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:I2CBUS:  
DTRACE?  
<x> = 1 or 2  
<NRf> = 1 to 8

Example :ANALYSIS:SBUS1:ANALYZE:I2CBUS:DTRACE 1  
:ANALYSIS:SBUS1:ANALYZE:I2CBUS:  
DTRACE? ->  
:ANALYSIS:SBUS1:ANALYZE:I2CBUS:  
DTRACE 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:LIST?**

Function Queries all settings related to the list display of the serial bus signal analysis.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:LIST?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:LIST? ->  
:ANALYSIS:SBUS1:ANALYZE:LIST:  
MODE DETAIL;SCROLL HORIZONTAL

**:ANALYSIS:SBUS<x>[:ANALYZE]:LIST:****ITEM?**

Function Queries the item in the list display of the serial bus signal analysis.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:LIST:ITEM?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:LIST:ITEM? ->  
:ANALYSIS:SBUS1:ANALYZE:LIST:ITEM  
"No., S/P, Hex, Form, R/W, ACK, "

**:ANALYSIS:SBUS<x>[:ANALYZE]:LIST:****MODE**

Function Sets the mode of the list display of the serial bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:LIST:  
MODE {DETAIL|SIMPLE}  
:ANALYSIS:SBUS<x>[:ANALYZE]:LIST:MODE?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:LIST:  
MODE DETAIL  
:ANALYSIS:SBUS1:ANALYZE:LIST:MODE? ->  
:ANALYSIS:SBUS1:ANALYZE:LIST:  
MODE DETAIL

## 4.2 ANALYSIS Group

### **:ANALYSIS:SBUS<x>[:ANALYZE]:LIST:**

#### **SCROLL**

**Function** Sets the scroll method of the list display of the serial bus signal analysis or queries the current setting.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:  
LIST:SCROLL {HORIZONTAL|VERTICAL}  
:ANALYSIS:SBUS<x>[:ANALYZE]:  
LIST:SCROLL?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1:ANALYZE:LIST:  
SCROLL HORIZONTAL  
:ANALYSIS:SBUS1:ANALYZE:LIST:SCROLL? ->  
:ANALYSIS:SBUS1:ANALYZE:LIST:  
SCROLL HORIZONTAL

### **:ANALYSIS:SBUS<x>[:ANALYZE]:LIST:VALUE?**

**Function** Queries the automated measured value of the specified analysis number in the analysis result list of the serial bus signal analysis.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:LIST:VALUE?  
{<NRf>|MAXIMUM|MINIMUM}  
<x> = 1, 2  
<NRf> = -40000 to 40000  
(<NRf> = -2999 to 2999 for :ANALYSIS:SBUS<x>  
[:ANALYZE]:MODE CANBUS)

**Example** :ANALYSIS:SBUS1:ANALYZE:LIST:  
VALUE? 1 ->  
:ANALYSIS:SBUS1:ANALYZE:LIST:  
VALUE "1, P, 00, A, , 0,"

**Description** Set the data to MAXIMUM or MINIMUM to specify the maximum list display number or the minimum list display number.

### **:ANALYSIS:SBUS<x>[:ANALYZE]:MODE**

**Function** Sets the serial bus signal analysis mode or queries the current setting.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:  
MODE {CANBUS|I2CBUS|SPIBUS}  
:ANALYSIS:SBUS<x>[:ANALYZE]:MODE?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1:ANALYZE:MODE I2CBUS  
:ANALYSIS:SBUS1:ANALYZE:MODE? ->  
:ANALYSIS:SBUS1:ANALYZE:MODE I2CBUS

### **:ANALYSIS:SBUS<x>[:ANALYZE]:RPOINT**

**Function** Sets the analysis reference point of the serial bus signal analysis or queries the current setting.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:  
RPOINT {MANUAL,<NRf>|TRIGGER}  
:ANALYSIS:SBUS<x>[:ANALYZE]:RPOINT?  
<x> = 1, 2  
<NRf> = -5 to 5 (div)

**Example** :ANALYSIS:SBUS1:ANALYZE:RPOINT MANUAL,1  
:ANALYSIS:SBUS1:ANALYZE:RPOINT? ->  
:ANALYSIS:SBUS1:ANALYZE:RPOINT MANUAL,  
1.00000E+00

### **:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS?**

**Function** Queries all settings related to the SPI bus signal analysis.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1:ANALYZE:SPIBUS? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CLOCK:  
POLARITY FALL;SOURCE 1;:ANALYSIS:SBUS1:  
ANALYZE:SPIBUS:CS:ACTIVE HIGH;TRACE 1;:  
ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:  
ACTIVE HIGH;TRACE 1;:ANALYSIS:SBUS1:  
ANALYZE:SPIBUS:DATA2:ACTIVE HIGH;  
TRACE 1;:ANALYSIS:SBUS1:ANALYZE:SPIBUS:  
SETUP:BITORDER LSBFIRST;MODE WIRE3

### **:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:**

#### **CLOCK?**

**Function** Queries all settings related to the clock channel of the SPI bus signal analysis.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:  
CLOCK?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1:ANALYZE:SPIBUS:CLOCK?  
-> :ANALYSIS:SBUS1:ANALYZE:SPIBUS:  
CLOCK:POLARITY FALL;SOURCE 1

### **:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:**

#### **CLOCK:POLARITY**

**Function** Sets the polarity of the clock channel of the SPI bus signal analysis or queries the current setting.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:  
CLOCK:POLARITY {FALL|RISE}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:  
CLOCK:POLARITY?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1:ANALYZE:SPIBUS:  
CLOCK:POLARITY FALL  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CLOCK:  
POLARITY? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CLOCK:  
POLARITY FALL

**:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CLOCK:SOURCE**

Function Sets the clock channel of the SPI bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CLOCK:SOURCE {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CLOCK:SOURCE?  
<x> = 1 or 2  
<NRf> = 1 to 8

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:CLOCK:SOURCE 1  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CLOCK:SOURCE? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CLOCK:SOURCE 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS?**

Function Queries all settings related to the chip select channel of the SPI bus signal analysis.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:ACTIVE HIGH;TRACE 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS:ACTIVE**

Function Sets the active level of the chip select channel of the SPI bus signal analysis or queries the current setting.

Syntax: ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS:ACTIVE {HIGH|LOW}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS:ACTIVE?  
<x> = 1 or 2

Example: :ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:ACTIVE HIGH  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:ACTIVE? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:ACTIVE HIGH

**:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS:TRACE**

Function Sets the chip select channel of the SPI bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS:TRACE {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:CS:TRACE?  
<x> = 1 or 2  
<NRf> = 1 to 8

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:TRACE 1  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:TRACE? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:CS:TRACE 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>?**

Function Queries all settings related to the data of the SPI bus signal analysis.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>?  
<x> of SBUS<x> = 1 or 2  
<x> of DATA<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:ACTIVE HIGH;TRACE 1

**:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>:ACTIVE**

Function Sets the active level of the data of the SPI bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>:ACTIVE {HIGH|LOW}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>:ACTIVE?  
<x> of SBUS<x> = 1 or 2  
<x> of DATA<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:ACTIVE HIGH  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:ACTIVE? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:ACTIVE HIGH

## 4.2 ANALYSIS Group

### **:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>:TRACE**

Function Sets the data channel of the SPI bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>:TRACE {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:DATA<x>:TRACE?  
<x> of SBUS<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<NRf> = 1 to 8

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:TRACE 1  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:TRACE? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:DATA1:TRACE 1

### **:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:SETUP?**

Function Queries all settings related to the SPI bus signal analysis setup.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS:SETUP?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP? -> :ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP:BITORDER LSBFIRST;MODE WIRE3

### **:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS[:SETUP]:BITORDER**

Function Sets the bit order of the SPI bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS[:SETUP]:BITORDER {LSBFIRST|MSBFIRST}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS[:SETUP]:BITORDER?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP:BITORDER LSBFIRST  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP:BITORDER? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP:BITORDER LSBFIRST

### **:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS[:SETUP]:MODE**

Function Sets the wiring system of the SPI bus signal analysis (three-wire or four-wire) or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS[:SETUP]:MODE {WIRE3|WIRE4}  
:ANALYSIS:SBUS<x>[:ANALYZE]:SPIBUS[:SETUP]:MODE?  
<x> = 1 or 2

Example :ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP:MODE WIRE3  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP:MODE? ->  
:ANALYSIS:SBUS1:ANALYZE:SPIBUS:SETUP:MODE WIRE3

### **:ANALYSIS:SBUS<x>[:ANALYZE]:TRACE<x>?**

Function Queries all settings related to the threshold level of the source channel of the serial bus signal analysis.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:TRACE<x>?  
<x> of SBUS<x> = 1 or 2  
<x> of TRACE<x> = 1 to 8

Example :ANALYSIS:SBUS1:ANALYZE:TRACE1? ->  
:ANALYSIS:SBUS1:ANALYZE:TRACE1:HYSTERESIS 1.000E+00;LEVEL 1.000E+00

### **:ANALYSIS:SBUS<x>[:ANALYZE]:TRACE<x>:HYSTERESIS**

Function Sets the hysteresis of the threshold level of the source channel of the serial bus signal analysis or queries the current setting.

Syntax :ANALYSIS:SBUS<x>[:ANALYZE]:TRACE<x>:HYSTERESIS {<NRf>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:TRACE<x>:HYSTERESIS?  
<x> of SBUS<x> = 1 or 2  
<x> of TRACE<x> = 1 to 8  
<NRf> = 0 to 4 (div)

Example :ANALYSIS:SBUS1:ANALYZE:TRACE1:HYSTERESIS 1  
:ANALYSIS:SBUS1:ANALYZE:TRACE1:HYSTERESIS? ->  
:ANALYSIS:SBUS1:ANALYZE:TRACE1:HYSTERESIS 1.000E+00

**:ANALYSIS:SBUS<x>[:ANALYZE]:****TRACe<x>:LEVel**

**Function** Sets the level of the threshold level of the source channel of the serial bus signal analysis or queries the current setting.

**Syntax** :ANALYSIS:SBUS<x>[:ANALYZE]:TRACe<x>:  
LEVel {<NRf>|<Voltage>|<current>}  
:ANALYSIS:SBUS<x>[:ANALYZE]:TRACe<x>:  
LEVel?  
<x> of SBUS<x> = 1 or 2  
<x> of TRACe<x> = 1 to 8  
<NRf>, <Voltage>, and <Current> = See the *User's Manual (IM701310-01E)*.

**Example** :ANALYSIS:SBUS1:ANALYZE:TRACE1:  
LEVEL 1V  
:ANALYSIS:SBUS1:ANALYZE:TRACE1:LEVEL?  
-> :ANALYSIS:SBUS1:ANALYZE:TRACE1:  
LEVEL 1.000E+00

**:ANALYSIS:SBUS<x>:ZLINKage**

**Function** Sets the zoom link of the serial bus signal analysis or queries the current setting.

**Syntax** :ANALYSIS:SBUS<x>:ZLINKage {OFF|Z1|Z2}  
:ANALYSIS:SBUS<x>:ZLINKage?  
<x> = 1 or 2

**Example** :ANALYSIS:SBUS1:ZLINKAGE OFF  
:ANALYSIS:SBUS1:ZLINKAGE? -  
>:ANALYSIS:SBUS1:ZLINKAGE OFF

**:ANALYSIS:TYPE<x>**

**Function** Sets the analysis function type or queries the current setting.

**Syntax** :ANALYSIS:TYPE<x>  
{AHISTogram|FFT|SBUS|WPARAMeter|XY}  
:ANALYSIS:TYPE<x>?  
<x> = 1 or 2

**Example** :ANALYSIS:TYPE1 AHISTOGRAM  
:ANALYSIS:TYPE1? ->  
:ANALYSIS:TYPE1 AHISTOGRAM

## 4.3 MATH Group

### **:MATH<x>:OPERation**

**Function** Sets the operator or queries the current setting.

**Syntax** :MATH<x>:OPERation {(ECount|FILTer|INTEgral|MINus|MULTiple|PLUS|RCOunt|SBIT),<NRf>,<NRf>}:MATH<x>:OPERation?<x> = 1 to 8 (<x> = 1 to 4 only when you select {SBIT})<NRf> = 1 to 4

**Example** :MATH1:OPERATION  
FILTER,1:MATH1:OPERATION? ->  
:MATH1:OPERATION FILTER,1

**Description** For unary operators (ECount|FILTer|INTEgral|SBIT), select the target waveform using the first <NRf>.  
For binary operators (MINus|MULTiple|PLUS|RCOunt), select the target waveform of the first term using the first <NRf> and the target waveform of the second term using the second <NRf>.

### **:MATH<x>:SBIT?**

**Function** Queries all settings related to the stuff bit computation.

**Syntax** :MATH<x>:SBIT?<x> = 1 to 4

**Example** :MATH1:SBIT? ->  
:MATH1:SBIT:BRATE 1000000;  
HYSTERESIS 600.000E-03;  
LEVEL 0.0000000E+00;RECESSIVE HIGH

### **:MATH<x>:SBIT:BRATE**

**Function** Sets the bit rate (data transfer rate) of the stuff bit computation or queries the current setting.

**Syntax** :MATH<x>:SBIT:BRATE {<NRf>|USER,<NRf>}:MATH<x>:SBIT:BRATE?<x> = 1 to 4<NRf> = 83300, 125000, 250000, 500000, 1000000<NRf> of USER = See the *User's Manual (IM701310-01E)*.

**Example** :MATH1:SBIT:BRATE 83300  
:MATH1:SBIT:BRATE? ->  
:MATH1:SBIT:BRATE 83300

### **:MATH<x>:SBIT:HYSTEResis**

**Function** Sets the hysteresis of the stuff bit computation or queries the current setting.

**Syntax** :MATH<x>:SBIT:HYSTEResis {<NRf>}:MATH<x>:SBIT:HYSTEResis?<x> = 1 to 4<NRf> = 0 to 4(div)

**Example** :MATH1:SBIT:HYSTERESIS 1  
:MATH1:SBIT:HYSTERESIS? ->  
:MATH1:SBIT:HYSTERESIS 1.00000E+00

### **:MATH<x>:SBIT:LEVel**

**Function** Sets the threshold level of the stuff bit computation or queries the current setting.

**Syntax** :MATH<x>:SBIT:LEVel {<NRf>|<Voltage>|<Current>}:MATH<x>:SBIT:LEVel?<x> = 1 to 4<NRf>, <Voltage>, and <Current> = See the *User's Manual (IM701310-01E)*.

**Example** :MATH1:SBIT:LEVEL 1  
:MATH1:SBIT:LEVEL? ->  
:MATH1:SBIT:LEVEL 1.0000000E+00

### **:MATH<x>:SBIT:REcessive**

**Function** Sets the recessive level (bus level) of the stuff bit computation or queries the current setting.

**Syntax** :MATH<x>:SBIT:REcessive {HIGH|LOW}:MATH<x>:SBIT:REcessive?<x> = 1 to 4

**Example** :MATH1:SBIT:RECESSIVE HIGH  
:MATH1:SBIT:RECESSIVE? ->  
:MATH1:SBIT:RECESSIVE HIGH

### **:MATH<x>:SBIT:SPOint**

**Function** Sets the sample point of the stuff bit computation or queries the current setting.

**Syntax** :MATH<x>:SBIT:SPOint {<NRf>}:MATH<x>:SBIT:SPOint?<x> = 1 to 4<NRf> = 18.8 to 90.6(%)

**Example** :MATH1:SBIT:SPOINT 18.8  
:MATH1:SBIT:SPOINT? ->  
:MATH1:SBIT:SPOINT 18.8E+00



## 4.4 SEARCh Group

### SEARCh<x>:CANBus?

**Function** Queries all settings related to the CAN bus signal search.

**Syntax** :SEARCh<x>:CANBus?  
<x> = 1, 2

**Example** :SEARCH1:CANBUS? ->  
:SEARCH1:CANBUS:SETUP:ACK DONTCARE;  
BRATE 1000000;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "100101100101100001110100010100  
100001001101010111101011110111100";  
SIGN UNSIGN;:SEARCH1:CANBUS:SETUP:  
IDEXT:PATTERN"1100101101110000111011101  
1111";:SEARCH1:CANBUS:SETUP:IDSTD:  
PATTERN "0001111101";:SEARCH1:CANBUS:  
SETUP:MODE SOF;RECESSIVE HIGH;RTR DATA;  
SPOINT 62.5E+00;TRACE 1

### :SEARCh<x>:CANBus:SETUp?

**Function** Queries all settings related to the CAN bus signal search setup.

**Syntax** :SEARCh<x>:CANBus:SETUp?  
<x> = 1, 2

**Example** :SEARCH1:CANBUS:SETUP? ->  
:SEARCH1:CANBUS:SETUP:ACK DONTCARE;  
BRATE 1000000;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "100101100101100001110100010100  
100001001101010111101011110111100";  
SIGN UNSIGN;:SEARCH1:CANBUS:SETUP:  
IDEXT:PATTERN "110010110111000011101110  
1111";:SEARCH1:CANBUS:SETUP:IDSTD:  
PATTERN "0001111101";:SEARCH1:CANBUS:  
SETUP:MODE SOF;RECESSIVE HIGH;RTR DATA;  
SPOINT 62.5E+00;TRACE 1

### :SEARCh<x>:CANBus[:SETUp]:ACK

**Function** Sets the ACK condition of the CAN bus signal search or queries the current setting.

**Syntax** :SEARCh<x>:CANBus[:SETUp]:  
ACK {ACK|ACKBoth|DONTcare|NONack}  
:SEARCh<x>:CANBus[:SETUp]:ACK?  
<x> = 1, 2

**Example** :SEARCH1:CANBUS:SETUP:ACK ACK  
:SEARCH1:CANBUS:SETUP:ACK? ->  
:SEARCH1:CANBUS:SETUP:ACK ACK

### :SEARCh<x>:CANBus[:SETUp]:BRATE

**Function** Sets the bit rate (data transfer rate) of the CAN bus signal search or queries the current setting.

**Syntax** :SEARCh<x>:CANBus[:SETUp]:  
BRATE {<Nrf>|USER,<Nrf>}  
:SEARCh<x>:CANBus[:SETUp]:BRATE?  
<x> = 1, 2  
<Nrf> = 83300, 125000, 250000, 500000,  
1000000  
<Nrf> of USER = See the *User's Manual*  
(IM701310-01E).

**Example** :SEARCH1:CANBUS:SETUP:BRATE 83300  
:SEARCH1:CANBUS:SETUP:BRATE? ->  
:SEARCH1:CANBUS:SETUP:BRATE 83300

### :SEARCh<x>:CANBus[:SETUp]:DATA?

**Function** Queries all settings related to the CAN bus signal search data.

**Syntax** :SEARCh<x>:CANBus[:SETUp]:DATA?  
<x> = 1, 2

**Example** :SEARCH1:CANBUS:SETUP:DATA? ->  
:SEARCH1:CANBUS:SETUP:DATA:BORDER BIG;  
CONDITION TRUE;DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "100101100101100001110100010100  
100001001101010111101011110111100";  
SIGN UNSIGN

### :SEARCh<x>:CANBus[:SETUp]:DATA:BORDER

**Function** Sets the byte order of the CAN bus signal search data or queries the current setting.

**Syntax** :SEARCh<x>:CANBus[:SETUp]:DATA:  
BORDER {BIG|LITTLE}  
:SEARCh<x>:CANBus[:SETUp]:DATA:BORDER?  
<x> = 1, 2

**Example** :SEARCH1:CANBUS:SETUP:DATA:BORDER BIG  
:SEARCH1:CANBUS:SETUP:DATA:BORDER? ->  
:SEARCH1:CANBUS:SETUP:DATA:BORDER BIG

## 4.4 SEARCh Group

### **:SEARCh<x>:CANBus [ :SETup ] :DATA:**

#### **CONDition**

**Function** Sets the data condition of the CAN bus signal search or queries the current setting.

**Syntax** :SEARCh<x>:CANBus [ :SETup ] :DATA:  
CONDition {BETween|DONTcare|FALSE|  
GTHan|LTHan|ORANge|TRUE}  
:SEARCh<x>:CANBus [ :SETup ] :DATA:  
CONDition?  
<x> = 1, 2

**Example** :SEARCH1:CANBUS:SETUP:DATA:  
CONDITION BETWEEN  
:SEARCH1:CANBUS:SETUP:DATA:CONDITION? ->  
:SEARCH1:CANBUS:SETUP:DATA:  
CONDITION BETWEEN

### **:SEARCh<x>:CANBus [ :SETup ] :DATA:DATA<x>**

**Function** Sets the comparison data of the CAN bus signal search data or queries the current setting.

**Syntax** :SEARCh<x>:CANBus [ :SETup ] :DATA:  
DATA<x> {<Nrf>}  
:SEARCh<x>:CANBus [ :SETup ] :DATA:DATA<x>?  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<Nrf> = See the *User's Manual (IM701310-01E)*.

**Example** :SEARCH1:CANBUS:SETUP:DATA:DATA1 1  
:SEARCH1:CANBUS:SETUP:DATA:DATA1? ->  
:SEARCH1:CANBUS:SETUP:DATA:  
DATA1 1.0000000E+00

**Description**

- Use :SEARCh<x>:CANBus [ :SETup ] :DATA: DATA1 when :SEARCh<x>:CANBus [ :SETup ] :DATA:CONDition GTHan is specified.
- Use :SEARCh<x>:CANBus [ :SETup ] :DATA: DATA2 when :SEARCh<x>:CANBus [ :SETup ] :DATA:CONDition LTHan is specified.
- Use :SEARCh<x>:CANBus [ :SETup ] :DATA: DATA1 to set the smaller value and :SEARCh<x>: CANBus [ :SETup ] :DATA:DATA2 to set the larger value when :SEARCh<x>:CANBus [ :SETup ] :DATA:CONDition BETWEEN|ORANge is specified.

### **:SEARCh<x>:CANBus [ :SETup ] :DATA:DLC**

**Function** Sets the number of valid bytes (DLC) of the CAN bus signal search data or queries the current setting.

**Syntax** :SEARCh<x>:CANBus [ :SETup ] :DATA:  
DLC {<Nrf>}  
:SEARCh<x>:CANBus [ :SETup ] :DATA:DLC?  
<x> = 1, 2  
<Nrf> = 0 to 8

**Example** :SEARCH1:CANBUS:SETUP:DATA:DLC 0  
:SEARCH1:CANBUS:SETUP:DATA:DLC? ->  
:SEARCH1:CANBUS:SETUP:DATA:DLC 0

### **:SEARCh<x>:CANBus [ :SETup ] :DATA:HEXA**

**Function** Sets the CAN bus signal search data in hexadecimal notation.

**Syntax** :SEARCh<x>:CANBus [ :SETup ] :DATA:  
HEXA {<String>}  
<x> = 1, 2  
<String> = Up to 16 characters by combining '0' to 'F' and 'X' (in one-byte unit)

**Example** :SEARCH1:CANBUS:SETUP:DATA:HEXA "A9"

### **:SEARCh<x>:CANBus [ :SETup ] :DATA:MSBLsb**

**Function** Sets the MSB and LSB bits of the CAN bus signal search data or queries the current setting.

**Syntax** :SEARCh<x>:CANBus [ :SETup ] :DATA:  
MSBLsb {<Nrf>,<Nrf>}  
:SEARCh<x>:CANBus [ :SETup ] :DATA:MSBLsb?  
<x> = 1, 2  
<Nrf> = See the *User's Manual (IM701310-01E)*.

**Example** :SEARCH1:CANBUS:SETUP:DATA:MSBLSB 1,0  
:SEARCH1:CANBUS:SETUP:DATA:MSBLSB? ->  
:SEARCH1:CANBUS:SETUP:DATA:MSBLSB 1,0

### **:SEARCh<x>:CANBus [ :SETup ] :DATA:PATtern**

**Function** Sets the CAN bus signal search data in binary notation or queries the current setting.

**Syntax** :SEARCh<x>:CANBus [ :SETup ] :DATA:  
PATtern {<String>}  
:SEARCh<x>:CANBus [ :SETup ] :DATA:PATtern?  
<x> = 1, 2  
<String> = Up to 64 characters by combining '0','1,' and 'X' (in one-byte unit)

**Example** :SEARCH1:CANBUS:SETUP:DATA:  
PATTERN "11011111"  
:SEARCH1:CANBUS:SETUP:DATA:PATTERN? ->  
:SEARCH1:CANBUS:SETUP:DATA:  
PATTERN "11011111"

### **:SEARCh<x>:CANBus [ :SETup ] :DATA:SIGN**

**Function** Sets the sign of the CAN bus signal search data or queries the current setting.

**Syntax** :SEARCh<x>:CANBus [ :SETup ] :DATA:  
SIGN {SIGN|UNSign}  
:SEARCh<x>:CANBus [ :SETup ] :DATA:SIGN?  
<x> = 1, 2

**Example** :SEARCH1:CANBUS:SETUP:DATA:SIGN SIGN  
:SEARCH1:CANBUS:SETUP:DATA:SIGN? ->  
:SEARCH1:CANBUS:SETUP:DATA:SIGN SIGN

**:SEARCh<x>:CANBus [ :SETUp ] :IDEXt?**

Function Queries all settings related to the ID of the extended format of the CAN bus signal search.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :IDEXt?  
<x> = 1, 2

Example :SEARCH1:CANBUS:SETUP:IDEXT? ->  
:SEARCH1:CANBUS:SETUP:IDEXT:  
PATTERN "11001011011100001110111011111"

**:SEARCh<x>:CANBus [ :SETUp ] :IDEXt:HEXA**

Function Sets the ID of the extended format of the CAN bus signal search in hexadecimal notation.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :IDEXt:  
HEXA {<String>}  
<x> = 1, 2

<String> = 8 characters by combining '0' to 'F' and 'X'  
Example :SEARCH1:CANBUS:SETUP:IDEXT:  
HEXA "1AEF5906"

**:SEARCh<x>:CANBus [ :SETUp ] :IDEXt:****PATtern**

Function Sets the ID of the extended format of the CAN bus signal search in binary notation or queries the current setting.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :IDEXt:  
PATtern {<String>}  
:SEARCh<x>:CANBus [ :SETUp ] :IDEXt:  
PATtern?  
<x> = 1, 2

<String> = 29 characters by combining '0', '1,' and 'X'  
Example :SEARCH1:CANBUS:SETUP:IDEXT:  
PATTERN "11001011011100001110111011111"  
:SEARCH1:CANBUS:SETUP:IDEXT:PATTERN? ->  
:SEARCH1:CANBUS:SETUP:IDEXT:  
PATTERN "11001011011100001110111011111"

**:SEARCh<x>:CANBus [ :SETUp ] :IDSTd?**

Function Queries all settings related to the ID of the standard format of the CAN bus signal search.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :IDSTd?  
<x> = 1, 2

Example :SEARCH1:CANBUS:SETUP:IDSTD? ->  
:SEARCH1:CANBUS:SETUP:IDSTD:  
PATTERN "00011111101"

**:SEARCh<x>:CANBus [ :SETUp ] :IDSTd:HEXA**

Function Sets the ID of the standard format of the CAN bus signal search in hexadecimal notation.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :IDSTd:  
HEXA {<String>}  
<x> = 1, 2

<String> = 3 characters by combining '0' to 'F' and 'X'  
Example :SEARCH1:CANBUS:SETUP:IDSTD:HEXA "5DF"

**:SEARCh<x>:CANBus [ :SETUp ] :IDSTd:****PATtern**

Function Sets the ID of the standard format of the CAN bus signal search in binary notation or queries the current setting.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :IDSTd:  
PATtern {<String>}  
:SEARCh<x>:CANBus [ :SETUp ] :IDSTd:  
PATtern?  
<x> = 1, 2

<String> = 11 characters by combining '0', '1,' and 'X'  
Example :SEARCH1:CANBUS:SETUP:IDSTD:  
PATTERN "10111011111"  
:SEARCH1:CANBUS:SETUP:IDSTD:PATTERN? ->  
:SEARCH1:CANBUS:SETUP:IDSTD:  
PATTERN "10111011111"

**:SEARCh<x>:CANBus [ :SETUp ] :MODE**

Function Sets the CAN bus signal search mode or queries the current setting.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :  
MODE {EFrame | IDExt | IDStd | SOF}  
:SEARCh<x>:CANBus [ :SETUp ] :MODE?  
<x> = 1, 2

Example :SEARCH1:CANBUS:SETUP:MODE EFRAME  
:SEARCH1:CANBUS:SETUP:MODE? ->  
:SEARCH1:CANBUS:SETUP:MODE EFRAME

**:SEARCh<x>:CANBus [ :SETUp ] :REcessive**

Function Sets the recessive level (bus level) of the CAN bus signal search or queries the current setting.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :  
REcessive {HIGH | LOW}  
:SEARCh<x>:CANBus [ :SETUp ] :REcessive?  
<x> = 1, 2

Example :SEARCH1:CANBUS:SETUP:RECESSIVE HIGH  
:SEARCH1:CANBUS:SETUP:RECESSIVE? ->  
:SEARCH1:CANBUS:SETUP:RECESSIVE HIGH

**:SEARCh<x>:CANBus [ :SETUp ] :RTR**

Function Sets the RTR of the CAN bus signal search or queries the current setting.

Syntax :SEARCh<x>:CANBus [ :SETUp ] :  
RTR {DATA | DONTcare | REMote}  
:SEARCh<x>:CANBus [ :SETUp ] :RTR?  
<x> = 1, 2

Example :SEARCH1:CANBUS:SETUP:RTR DATA  
:SEARCH1:CANBUS:SETUP:RTR? ->  
:SEARCH1:CANBUS:SETUP:RTR DATA

## 4.4 SEARCh Group

### **:SEARCh<x>:CANBus [ :SETup ] :SPOint**

Function Sets the sample point of the CAN bus signal search or queries the current setting.

Syntax :SEARCh<x>:CANBus [ :SETup ] :  
SPOint {<NRf>}  
:SEARCh<x>:CANBus [ :SETup ] :SPOint?  
<x> = 1, 2  
<NRf>=18.8 to 90.6(%)

Example :SEARCH1:CANBUS:SETUP:SPOINT 18.8  
:SEARCH1:CANBUS:SETUP:SPOINT? ->  
:SEARCH1:CANBUS:SETUP:SPOINT 18.8E+00

### **:SEARCh<x>:CANBus [ :SETup ] :TRACe**

Function Sets the trace of the CAN bus signal search or queries the current setting.

Syntax :SEARCh<x>:CANBus [ :SETup ] :TRACe {<NRf>}  
:SEARCh<x>:CANBus [ :SETup ] :TRACe?  
<x> = 1, 2  
<NRf> = 1 to 8

Example :SEARCH1:CANBUS:SETUP:TRACE 1  
:SEARCH1:CANBUS:SETUP:TRACE? ->  
:SEARCH1:CANBUS:SETUP:TRACE 1

### **SEARCh<x>:I2CBus?**

Function Queries all settings related to the I<sup>2</sup>C bus signal search.

Syntax :SEARCh<x>:I2CBus?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS? ->  
:SEARCH1:I2CBUS:CLOCK:SOURCE 1;  
:SEARCH1:I2CBUS:SETUP:ADATA:  
BIT10ADDRESS:PATTERN "10111011111";  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7ADDRESS:  
PATTERN "11011110";:SEARCH1:I2CBUS:  
SETUP:ADATA:BIT7APSUB:ADDRESS:  
PATTERN "11001101";:SEARCH1:I2CBUS:  
SETUP:ADATA:BIT7APSUB:SADDRESS:  
PATTERN "11101111";:SEARCH1:I2CBUS:  
SETUP:ADATA:TYPE BIT7APSUB;:SEARCH1:  
I2CBUS:SETUP:DATA:BYTE 1;  
CONDITION TRUE;DPOSITION 0;MODE 0;  
PATTERN1 "10101011";  
PATTERN2 "10101011";  
PATTERN3 "10101011";  
PATTERN4 "10101011";  
PMODE DONTCARE;:SEARCH1:I2CBUS:SETUP:  
GCALL:BIT7MADDRESS:PATTERN "1010101";:  
:SEARCH1:I2CBUS:SETUP:GCALL:  
SBYTE BIT7MADDRESS;:SEARCH1:I2CBUS:  
SETUP:MODE SBHSMODE;.....

### **:SEARCh<x>:I2CBus:CLOCK?**

Function Queries all settings related to the clock of the I<sup>2</sup>C bus signal search.

Syntax :SEARCh<x>:I2CBus:CLOCK?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:CLOCK? ->  
:SEARCH1:I2CBUS:CLOCK:SOURCE 1

### **:SEARCh<x>:I2CBus:CLOCK:SOURCE**

Function Sets the clock trace of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus:CLOCK:SOURCE {<NRf>}  
:SEARCh<x>:I2CBus:CLOCK:SOURCE?  
<x> = 1 or 2  
<NRf> = 1 to 8

Example :SEARCH1:I2CBUS:CLOCK:SOURCE 1  
:SEARCH1:I2CBUS:CLOCK:SOURCE? ->  
:SEARCH1:I2CBUS:CLOCK:SOURCE 1

### **:SEARCh<x>:I2CBus:SETup?**

Function Queries all settings related to the I<sup>2</sup>C bus signal search setup.

Syntax :SEARCh<x>:I2CBus:SETup?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:  
BIT10ADDRESS:PATTERN "10111011111";:  
:SEARCH1:I2CBUS:SETUP:ADATA:  
BIT7ADDRESS:PATTERN "11011110";:  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN "11001101";:SEARCH1:  
I2CBUS:SETUP:ADATA:BIT7APSUB:  
SADDRESS:PATTERN "11101111";:SEARCH1:  
I2CBUS:SETUP:ADATA:TYPE BIT7APSUB;:  
:SEARCH1:I2CBUS:SETUP:DATA:BYTE 1;  
CONDITION TRUE;DPOSITION 0;MODE 0;  
PATTERN1 "10101011";  
PATTERN2 "10101011";  
PATTERN3 "10101011";  
PATTERN4 "10101011";PMODE DONTCARE;:  
:SEARCH1:I2CBUS:SETUP:GCALL:  
BIT7MADDRESS:PATTERN "1010101";:  
:SEARCH1:I2CBUS:SETUP:GCALL:  
SBYTE BIT7MADDRESS;:SEARCH1:I2CBUS:  
SETUP:MODE SBHSMODE;NAIGNORE:HSMODE 0;  
RACCESS 0;SBYTE 0;:SEARCH1:I2CBUS:  
SETUP:SBHSMODE:TYPE SBYTE

**:SEARCh<x>:I2CBUS[:SETup]:ADATa?**

**Function** Queries all settings related to the address of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBUS[:SETup]:ADATa?  
<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:ADATa? ->  
:SEARCH1:I2CBUS:SETUP:ADATa:  
BIT10ADDRESS:PATTERN "10111011111";:  
SEARCH1:I2CBUS:SETUP:ADATa:  
BIT7ADDRESS:PATTERN "11011110";:  
SEARCH1:I2CBUS:SETUP:ADATa:  
BIT7APSUB:ADDRESS:PATTERN "11001101";:  
SEARCH1:I2CBUS:SETUP:ADATa:BIT7APSUB:  
SADDRESS:PATTERN "11101111";:  
SEARCH1:I2CBUS:SETUP:ADATa:  
TYPE BIT7APSUB

**:SEARCh<x>:I2CBUS[:SETup]:ADATa:BIT10address?**

**Function** Queries all settings related to the 10-bit address of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBUS[:SETup]:ADATa:  
BIT10address?  
<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:  
ADATa:BIT10ADDRESS? ->  
:SEARCH1:I2CBUS:SETUP:ADATa:  
BIT10ADDRESS:PATTERN "00011111101"

**:SEARCh<x>:I2CBUS[:SETup]:ADATa:BIT10address:HEXA**

**Function** Sets the 10-bit address of the I<sup>2</sup>C bus signal search in hexadecimal notation.

**Syntax** :SEARCh<x>:I2CBUS[:SETup]:ADATa:  
BIT10address:HEXA {<String>}  
<x> = 1 or 2  
<String> = 3 characters by combining '0' to 'F' and 'X' (bit 8 is the R/W bit)

**Example** :SEARCH1:I2CBUS:SETUP:ADATa:  
BIT10ADDRESS:HEXA "5DF"

**:SEARCh<x>:I2CBUS[:SETup]:ADATa:BIT10address:PATtern**

**Function** Sets the 10-bit address of the I<sup>2</sup>C bus signal search in binary notation or queries the current setting.

**Syntax** :SEARCh<x>:I2CBUS[:SETup]:ADATa:  
BIT10address:PATtern {<String>}  
:SEARCh<x>:I2CBUS[:SETup]:ADATa:  
BIT10address:PATtern?  
<x> = 1 or 2  
<String> = 11 characters by combining '0', '1', and 'X' (bit 8 is the R/W bit)

**Example** :SEARCH1:I2CBUS:SETUP:ADATa:  
BIT10ADDRESS:PATTERN "10111011111"  
:SEARCH1:I2CBUS:SETUP:ADATa:  
BIT10ADDRESS:PATTERN? ->  
:SEARCH1:I2CBUS:SETUP:ADATa:  
BIT10ADDRESS:PATTERN "10111011111"

**:SEARCh<x>:I2CBUS[:SETup]:ADATa:BIT7Address?**

**Function** Queries all settings related to the 7-bit address of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBUS[:SETup]:ADATa:  
BIT7Address?  
<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:ADATa:  
BIT7ADDRESS? ->  
:SEARCH1:I2CBUS:SETUP:ADATa:  
BIT7ADDRESS:PATTERN "11011110"

**:SEARCh<x>:I2CBUS[:SETup]:ADATa:BIT7Address:HEXA**

**Function** Sets the 7-bit address of the I<sup>2</sup>C bus signal search in hexadecimal notation.

**Syntax** :SEARCh<x>:I2CBUS[:SETup]:ADATa:  
BIT7Address:HEXA {<String>}  
<x> = 1 or 2  
<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is the R/W bit)

**Example** :SEARCH1:I2CBUS:SETUP:ADATa:  
BIT7ADDRESS:HEXA "DE"

## 4.4 SEARCh Group

### **:SEARCh<x>:I2CBus[:SETup]:ADATa:**

#### **BIT7ADdress: PATTern**

**Function** Sets the 7-bit address of the I<sup>2</sup>C bus signal search in binary notation or queries the current setting.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7ADdress: PATTern {<String>}  
:SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7ADdress: PATTern?  
<x> = 1 or 2  
<String> = 8 characters by combining '0', '1', and 'X'  
(bit 0 is the R/W bit)

**Example** :SEARCH1:I2CBUS:SETUP:ADATA:  
BIT7ADDRESS:PATTERN "11011110"  
:SEARCH1:I2CBUS:SETUP:ADATA:  
BIT7ADDRESS:PATTERN? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:  
BIT7ADDRESS:PATTERN "11011110"

### **:SEARCh<x>:I2CBus[:SETup]:ADATa:**

#### **BIT7APsub?**

**Function** Queries all settings related to the 7-bit + Sub address of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub?  
<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN "11001101";:SEARCH1:  
I2CBUS:SETUP:ADATA:BIT7APSUB:  
SADDRESS:PATTERN "11101111"

### **:SEARCh<x>:I2CBus[:SETup]:ADATa:**

#### **BIT7APsub: ADDRESS?**

**Function** Queries all settings related to the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub: ADDRESS?  
<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN "11001101"

### **:SEARCh<x>:I2CBus[:SETup]:ADATa:**

#### **BIT7APsub: ADDRESS: HEXA**

**Function** Sets the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal search in hexadecimal notation.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub: ADDRESS: HEXA {<String>}  
<x> = 1 or 2  
<String> = 2 characters by combining '0' to 'F' and 'X'  
(bit 0 is the R/W bit)

**Example** :SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:HEXA "CD"

### **:SEARCh<x>:I2CBus[:SETup]:ADATa:**

#### **BIT7APsub: ADDRESS: PATTern**

**Function** Sets the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal search in binary notation or queries the current setting.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub: ADDRESS: PATTern {<String>}  
:SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub: ADDRESS: PATTern?  
<x> = 1 or 2  
<String> = 8 characters by combining '0', '1', and 'X'  
(bit 0 is the R/W bit)

**Example** :SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN "11001101"  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN "11001101"

### **:SEARCh<x>:I2CBus[:SETup]:ADATa:**

#### **BIT7APsub: SADDRESS?**

**Function** Queries all settings related to the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub: SADDRESS?  
<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
SADDRESS? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
SADDRESS:PATTERN "11101111"

### **:SEARCh<x>:I2CBus[:SETup]:ADATa:**

#### **BIT7APsub: SADDRESS: HEXA**

**Function** Sets the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal search in hexadecimal notation.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub: SADDRESS: HEXA {<String>}  
<x> = 1 or 2  
<String> = 2 characters by combining '0' to 'F' and 'X'

**Example** :SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
SADDRESS:HEXA "EF"

**:SEARCh<x>:I2CBus[:SETup]:ADATa:****BIT7APsub:SADdress:PATtern**

Function Sets the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal search in binary notation or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub:SADdress:PATtern {<String>}  
:SEARCh<x>:I2CBus[:SETup]:ADATa:  
BIT7APsub:SADdress:PATtern?  
<x> = 1 or 2  
<String> = 8 characters by combining '0,' '1,' and 'X'

Example :SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN "11101111"  
:SEARCH1:I2CBUS:SETUP:ADATA:BIT7APSUB:  
ADDRESS:PATTERN? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:  
BIT7APSUB:SADDRESS:PATTERN "11101111"

**:SEARCh<x>:I2CBus[:SETup]:ADATa:TYPE**

Function Sets the address type of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:ADATa:  
TYPE {BIT10address|BIT7ADdress|  
BIT7APsub}  
:SEARCh<x>:I2CBus[:SETup]:ADATa:TYPE?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:ADATA:  
TYPE BIT10ADDRESS  
:SEARCH1:I2CBUS:SETUP:ADATA:TYPE? ->  
:SEARCH1:I2CBUS:SETUP:ADATA:  
TYPE BIT10ADDRESS

**:SEARCh<x>:I2CBus[:SETup]:DATA?**

Function Queries all settings related to the data of the I<sup>2</sup>C bus signal search.

Syntax :SEARCh<x>:I2CBus[:SETup]:DATA?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:DATA? ->  
:SEARCH1:I2CBUS:SETUP:DATA:BYTE 1;  
CONDITION TRUE;DPOSITION 0;MODE 0;  
PATTERN1 "10101011";  
PATTERN2 "10101011";  
PATTERN3 "10101011";  
PATTERN4 "10101011";PMODE DONTCARE

**:SEARCh<x>:I2CBus[:SETup]:DATA:BYTE**

Function Sets the number of data bytes of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:DATA:  
BYTE {<Nrf>}  
:SEARCh<x>:I2CBus[:SETup]:DATA:BYTE?  
<x> = 1 or 2  
<Nrf> = 1 to 4

Example :SEARCH1:I2CBUS:SETUP:DATA:BYTE 1  
:SEARCH1:I2CBUS:SETUP:DATA:BYTE? ->  
:SEARCH1:I2CBUS:SETUP:DATA:BYTE 1

**:SEARCh<x>:I2CBus[:SETup]:DATA:****CONDition**

Function Sets the determination method (match or not match) of the data of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:DATA:  
CONDition {FALSE|TRUE}  
:SEARCh<x>:I2CBus[:SETup]:DATA:  
CONDition?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:DATA:  
CONDITION TRUE  
:SEARCH1:I2CBUS:SETUP:DATA:  
CONDITION? ->  
:SEARCH1:I2CBUS:SETUP:DATA:  
CONDITION TRUE

**:SEARCh<x>:I2CBus[:SETup]:DATA:****DPOSITION**

Function Sets the position for comparing the data pattern of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:DATA:  
DPOSITION {<Nrf>}  
:SEARCh<x>:I2CBus[:SETup]:DATA:  
DPOSITION?  
<x> = 1 or 2  
<Nrf> = 0 to 9999

Example :SEARCH1:I2CBUS:SETUP:DATA:DPOSITION 1  
:SEARCH1:I2CBUS:SETUP:DATA:  
DPOSITION? ->  
:SEARCH1:I2CBUS:SETUP:DATA:DPOSITION 1

**:SEARCh<x>:I2CBus[:SETup]:DATA:****HEXA<x>**

Function Sets the data of the I<sup>2</sup>C bus signal search in hexadecimal notation.

Syntax :SEARCh<x>:I2CBus[:SETup]:DATA:  
HEXA<x> {<String>}  
<x> of SEARCh<x> = 1 or 2  
<x> of HEXA<x> = 1 to 4  
<String> = 2 characters by combining '0' to 'F' and 'X'

Example :SEARCH1:I2CBUS:SETUP:DATA:HEXA1 "AB"

**:SEARCh<x>:I2CBus[:SETup]:DATA:MODE**

Function Enables/Disables the data conditions of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:DATA:  
MODE {<Boolean>}  
:SEARCh<x>:I2CBus[:SETup]:DATA:MODE?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:DATA:MODE ON  
:SEARCH1:I2CBUS:SETUP:DATA:MODE? ->  
:SEARCH1:I2CBUS:SETUP:DATA:MODE 1

## 4.4 SEARCh Group

### **:SEARCh<x>:I2CBus[:SETup]:DATA:**

#### **PATTErn<x>**

**Function** Sets the data of the I<sup>2</sup>C bus signal search in binary notation or queries the current setting.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:DATA:

PATTErn<x> {<String>}

:SEARCh<x>:I2CBus[:SETup]:DATA:

PATTErn<x>?

<x> of SEARCh<x> = 1 or 2

<x> of <PATTErn x> = 1 to 4

<String> = 8 characters by combining '0', '1,' and 'X'

**Example** :SEARCH1:I2CBUS:SETUP:DATA:

PATTERN1 "10101011"

:SEARCH1:I2CBUS:SETUP:DATA:PATTERN1?

-> :SEARCH1:I2CBUS:SETUP:DATA:

PATTERN1 "10101011"

### **:SEARCh<x>:I2CBus[:SETup]:DATA:PMODE**

**Function** Sets the pattern comparison start position mode of the data of the I<sup>2</sup>C bus signal search or queries the current setting.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:DATA:

PMODE {DONTcare|SELEct}

:SEARCh<x>:I2CBus[:SETup]:DATA:PMODE?

<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:DATA:

PMODE DONTCARE

:SEARCH1:I2CBUS:SETUP:DATA:PMODE? ->

:SEARCH1:I2CBUS:SETUP:DATA:

PMODE DONTCARE

### **:SEARCh<x>:I2CBus[:SETup]:GCALl?**

**Function** Queries all settings related to the general call of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:GCALl?

<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:GCALL? ->

:SEARCH1:I2CBUS:SETUP:GCALL:

BIT7MADDRESS:PATTERN "1010101";;

SEARCH1:I2CBUS:SETUP:GCALL:

SBYTE BIT7MADDRESS

### **:SEARCh<x>:I2CBus[:SETup]:GCALl:**

#### **BIT7maddress?**

**Function** Queries all settings related to the 7-bit master address of the general call of the I<sup>2</sup>C bus signal search.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:GCALl:

BIT7maddress?

<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:GCALL:

BIT7MADDRESS? ->

:SEARCH1:I2CBUS:SETUP:GCALL:

BIT7MADDRESS:PATTERN "1010101"

### **:SEARCh<x>:I2CBus[:SETup]:GCALl:**

#### **BIT7maddress:HEXA**

**Function** Sets the 7-bit master address of the general call of the I<sup>2</sup>C bus signal search in hexadecimal notation.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:GCALl:

BIT7maddress:HEXA {<String>}

<x> = 1 or 2

<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is fixed 1)

**Example** :SEARCH1:I2CBUS:SETUP:GCALL:

BIT7MADDRESS:HEXA "BA"

### **:SEARCh<x>:I2CBus[:SETup]:GCALl:**

#### **BIT7maddress:PATTErn**

**Function** Sets the 7-bit master address of the general call of the I<sup>2</sup>C bus signal search in binary notation or queries the current setting.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:GCALl:

BIT7maddress:PATTErn {<String>}

:SEARCh<x>:I2CBus[:SETup]:GCALl:

BIT7maddress:PATTErn?

<x> = 1 or 2

<String> = 7 characters by combining '0', '1,' and 'X'

**Example** :SEARCH1:I2CBUS:SETUP:GCALL:

BIT7MADDRESS:PATTERN "1010101"

:SEARCH1:I2CBUS:SETUP:GCALL:

BIT7MADDRESS:PATTERN? ->

:SEARCH1:I2CBUS:SETUP:GCALL:

BIT7MADDRESS:PATTERN "1010101"

### **:SEARCh<x>:I2CBus[:SETup]:GCALl:**

#### **SBYTE (Second Byte)**

**Function** Sets the second byte type of the general call of the I<sup>2</sup>C bus signal search or queries the current setting.

**Syntax** :SEARCh<x>:I2CBus[:SETup]:GCALl:

SBYTE {BIT7maddress|DONTcare|H04|H06}

:SEARCh<x>:I2CBus[:SETup]:GCALl:SBYTE?

<x> = 1 or 2

**Example** :SEARCH1:I2CBUS:SETUP:GCALL:

SBYTE BIT7MADDRESS

:SEARCH1:I2CBUS:SETUP:GCALL:SBYTE? ->

:SEARCH1:I2CBUS:SETUP:GCALL:

SBYTE BIT7MADDRESS



**:SEARCh<x>:I2CBus[:SETup]:MODE**

Function Sets the search mode of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:  
MODE {ADATa|ESTart|GCALl|NAIGNore|  
SBHSmode}  
:SEARCh<x>:I2CBus[:SETup]:MODE?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:MODE ADATA  
:SEARCH1:I2CBUS:SETUP:MODE? ->  
:SEARCH1:I2CBUS:SETUP:MODE ADATA

**:SEARCh<x>:I2CBus[:SETup]:NAIGNore?**

Function Queries all settings related to the NON ACK ignore mode of the I<sup>2</sup>C bus signal search.

Syntax :SEARCh<x>:I2CBus[:SETup]:NAIGNore?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:NAIGNORE? ->  
:SEARCH1:I2CBUS:SETUP:NAIGNORE:  
HSMODE 1;RACCESS 1;SBYTE 1

**:SEARCh<x>:I2CBus[:SETup]:NAIGNore:HSMode**

Function Sets whether to ignore NON ACK in high speed mode of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:NAIGNore:  
HSMode {<Boolean>}  
:SEARCh<x>:I2CBus[:SETup]:NAIGNore:  
HSMode?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:NAIGNORE:  
HSMODE ON  
:SEARCH1:I2CBUS:SETUP:NAIGNORE:HSMODE? ->  
:SEARCH1:I2CBUS:SETUP:NAIGNORE:HSMODE 1

**:SEARCh<x>:I2CBus[:SETup]:NAIGNore:RACCEss**

Function Sets whether to ignore NON ACK in read access mode of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:NAIGNore:  
RACCEss {<Boolean>}  
:SEARCh<x>:I2CBus[:SETup]:NAIGNore:  
RACCEss?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:NAIGNORE:  
RACCESS ON  
:SEARCH1:I2CBUS:SETUP:NAIGNORE:  
RACCESS? ->  
:SEARCH1:I2CBUS:SETUP:NAIGNORE:  
RACCESS 1

**:SEARCh<x>:I2CBus[:SETup]:NAIGNore:SBYTE(Start Byte)**

Function Sets whether to ignore NON ACK in the start byte of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:NAIGNore:  
SBYTE {<Boolean>}  
:SEARCh<x>:I2CBus[:SETup]:NAIGNore:  
SBYTE?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:NAIGNORE:SBYTE ON  
:SEARCH1:I2CBUS:SETUP:NAIGNORE:  
SBYTE? ->  
:SEARCH1:I2CBUS:SETUP:NAIGNORE:SBYTE 1

**:SEARCh<x>:I2CBus[:SETup]:SBHSmode?**

Function Queries all settings related to the start byte and high speed mode of the I<sup>2</sup>C bus signal search.

Syntax :SEARCh<x>:I2CBus[:SETup]:SBHSmode?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:SBHSMODE? ->  
:SEARCH1:I2CBUS:SETUP:SBHSMODE:  
TYPE HSMODE

**:SEARCh<x>:I2CBus[:SETup]:SBHSmode:TYPE**

Function Sets the type of the start byte or high speed mode of the I<sup>2</sup>C bus signal search or queries the current setting.

Syntax :SEARCh<x>:I2CBus[:SETup]:SBHSmode:  
TYPE {HSMode|SBYTE}  
:SEARCh<x>:I2CBus[:SETup]:SBHSmode:  
TYPE?  
<x> = 1 or 2

Example :SEARCH1:I2CBUS:SETUP:SBHSMODE:  
TYPE HSMODE  
:SEARCH1:I2CBUS:SETUP:SBHSMODE:TYPE? ->  
:SEARCH1:I2CBUS:SETUP:SBHSMODE:  
TYPE HSMODE

## 4.4 SEARCh Group

### **:SEARCh<x>:SPIBUS?**

Function Queries all settings related to the SPI bus signal search.

Syntax :SEARCh<x>:SPIBUS?  
<x> = 1 or 2

Example :SEARCH1:SPIBUS? ->  
:SEARCH1:SPIBUS:CLOCK:POLARITY FALL;  
SOURCE 1;:SEARCH1:SPIBUS:CS:  
ACTIVE HIGH;TRACE 1;:SEARCH1:SPIBUS:  
SETUP:BITORDER LSBFIRST;DATA1:BYTE 1;  
CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "01111000";TRACE 1;:SEARCH1:  
SPIBUS:SETUP:DATA2:BYTE 1;  
CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "01111000";TRACE 1;:SEARCH1:  
SPIBUS:SETUP:MODE WIRE3

### **:SEARCh<x>:SPIBUS:CLOCK**

Function Queries all settings related to the clock channel of the SPI bus signal search.

Syntax :SEARCh<x>:SPIBUS:CLOCK?  
<x> = 1 or 2

Example :SEARCH1:SPIBUS:CLOCK? ->  
:SEARCH1:SPIBUS:CLOCK:POLARITY FALL;  
SOURCE 1

### **:SEARCh<x>:SPIBUS:CLOCK:POLarity**

Function Sets the polarity of the clock channel of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS:CLOCK:  
POLarity {FALL|RISE}  
:SEARCh<x>:SPIBUS:CLOCK:POLarity?  
<x> = 1 or 2

Example :SEARCH1:SPIBUS:CLOCK:POLARITY FALL  
:SEARCH1:SPIBUS:CLOCK:POLARITY? ->  
:SEARCH1:SPIBUS:CLOCK:POLARITY FALL

### **:SEARCh<x>:SPIBUS:CLOCK:SOURce**

Function Sets the clock channel of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS:CLOCK:SOURce {<Nrf>}  
:SEARCh<x>:SPIBUS:CLOCK:SOURce?  
<x> = 1 or 2  
<Nrf> = 1 to 8

Example :SEARCH1:SPIBUS:CLOCK:SOURCE 1  
:SEARCH1:SPIBUS:CLOCK:SOURCE? ->  
:SEARCH1:SPIBUS:CLOCK:SOURCE 1

### **:SEARCh<x>:SPIBUS:CS?**

Function Queries all settings related to the chip select channel of the SPI bus signal search.

Syntax :SEARCh<x>:SPIBUS:CS?  
<x> = 1 or 2

Example :SEARCH1:SPIBUS:CS? ->  
:SEARCH1:SPIBUS:CS:ACTIVE HIGH;TRACE 1

### **:SEARCh<x>:SPIBUS:CS:ACTIve**

Function Sets the active level of the chip select channel of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS:CS:ACTIve {HIGH|LOW}  
:SEARCh<x>:SPIBUS:CS:ACTIve?  
<x> = 1 or 2

Example :SEARCH1:SPIBUS:CS:ACTIVE HIGH  
:SEARCH1:SPIBUS:CS:ACTIVE? ->  
:SEARCH1:SPIBUS:CS:ACTIVE HIGH

### **:SEARCh<x>:SPIBUS:CS:TRACe**

Function Sets the chip select channel of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS:CS:TRACe {<Nrf>}  
:SEARCh<x>:SPIBUS:CS:TRACe?  
<x> = 1 or 2  
<Nrf> = 1 to 8

Example :SEARCH1:SPIBUS:CS:TRACE 1  
:SEARCH1:SPIBUS:CS:TRACE? ->  
:SEARCH1:SPIBUS:CS:TRACE 1

### **:SEARCh<x>:SPIBUS:SETup?**

Function Queries all settings related to the SPI bus signal search setup.

Syntax :SEARCh<x>:SPIBUS:SETup?  
<x> = 1 or 2

Example :SEARCH1:SPIBUS:SETUP? ->  
:SEARCH1:SPIBUS:SETUP:  
BITORDER LSBFIRST;DATA1:BYTE 1;  
CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "01111000";TRACE 1;:SEARCH1:  
SPIBUS:SETUP:DATA2:BYTE 1;  
CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "01111000";TRACE 1;:SEARCH1:  
SPIBUS:SETUP:MODE WIRE3

**:SEARCh<x>:SPIBUS[:SETUP]:BITOrder**

Function Sets the bit order of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS[:SETUP]:  
BITOrder {LSBFirst|MSBFirst}  
:SEARCh<x>:SPIBUS[:SETUP]:BITOrder?  
<x> = 1 or 2

Example :SEARCH1:SPIBUS:SETUP:BITORDER LSBFIRST  
:SEARCH1:SPIBUS:SETUP:BITORDER? ->  
:SEARCH1:SPIBUS:SETUP:BITORDER LSBFIRST

**:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>?**

Function Queries all settings related to the data of the SPI bus signal search.

Syntax :SEARCh<x>:SPIBUS[:SETUP]:DATA<x>?  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2

Example :SEARCH1:SPIBUS:SETUP:DATA1? ->  
:SEARCH1:SPIBUS:SETUP:DATA1:BYTE 1;  
CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "01111000";TRACE 1

Description DATA2 is valid when :SEARCh<x>:  
SPIBUS[:SETUP]:MODE WIRE4 is specified.

**:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:BYTE**

Function Sets the number of bytes of the data of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
BYTE {<Nrf>}  
:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:BYTE?  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<Nrf> = 1 to 4

Example :SEARCH1:SPIBUS:SETUP:DATA1:BYTE 1  
:SEARCH1:SPIBUS:SETUP:DATA1:BYTE? ->  
:SEARCH1:SPIBUS:SETUP:DATA1:BYTE 1

**:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:****CONdITION**

Function Sets the determination method (match or not match) of the data of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
CONdITION {FALSE|TRUE}  
:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
CONdITION?  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2

Example :SEARCH1:SPIBUS:SETUP:DATA1:  
CONDITION TRUE  
:SEARCH1:SPIBUS:SETUP:DATA1:  
CONDITION? ->  
:SEARCH1:SPIBUS:SETUP:DATA1:  
CONDITION TRUE

**:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:****DPOSITION**

Function Sets the pattern comparison start position of the data of the SPI bus signal search or queries the current setting.

Syntax :SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
DPOSITION {<Nrf>}  
:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
DPOSITION?  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<Nrf> = 0 to 9999

Example :SEARCH1:SPIBUS:SETUP:DATA1:DPOSITION 1  
:SEARCH1:SPIBUS:SETUP:DATA1:  
DPOSITION? ->  
:SEARCH1:SPIBUS:SETUP:DATA1:DPOSITION 1

**:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:****HEXA<x>**

Function Sets the data of the SPI bus signal search in hexadecimal notation.

Syntax :SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
HEXA<x> {<String>}  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<x> of HEXA<x> = 1 to 4  
<String> = 2 characters by combining '0' to 'F' and 'X'

Example :SEARCH1:SPIBUS:SETUP:DATA1:HEXA1 "EF"

**:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:****PATtern<x>**

Function Sets the data of the SPI bus signal search in binary notation or queries the current setting.

Syntax :SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
PATtern<x> {<String>}  
:SEARCh<x>:SPIBUS[:SETUP]:DATA<x>:  
PATtern<x>?  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<x> of <PATtern x> = 1 to 4  
<String> = 8 characters by combining '0', '1,' and 'X'

Example :SEARCH1:SPIBUS:SETUP:DATA1:  
PATTERN1 "11101111"  
:SEARCH1:SPIBUS:SETUP:DATA1:  
PATTERN1? ->  
:SEARCH1:SPIBUS:SETUP:DATA1:  
PATTERN1 "11101111"

## 4.4 SEARCh Group

### **:SEARCh<x>:SPIBus [ :SETup ] :DATA<x>:**

#### **TRACe**

**Function** Sets the source channel of the data of the SPI bus signal search or queries the current setting.

**Syntax** :SEARCh<x>:SPIBus [ :SETup ] :DATA<x>:  
TRACe {<NRf>}  
:SEARCh<x>:SPIBus [ :SETup ] :DATA<x>:  
TRACe?  
<x> of SEARCh<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<NRf> = 1 to 8

**Example** :SEARCH1:SPIBUS:SETUP:DATA1:TRACE 1  
:SEARCH1:SPIBUS:SETUP:DATA1:TRACE? ->  
:SEARCH1:SPIBUS:SETUP:DATA1:TRACE 1

### **:SEARCh<x>:SPIBus [ :SETup ] :MODE**

**Function** Sets the wiring system of the SPI bus signal search (three-wire or four-wire) or queries the current setting.

**Syntax** :SEARCh<x>:SPIBus [ :SETup ] :  
MODE {WIRE3|WIRE4}  
:SEARCh<x>:SPIBus [ :SETup ] :MODE?  
<x> = 1 or 2

**Example** :SEARCH1:SPIBUS:SETUP:MODE WIRE3  
:SEARCH1:SPIBUS:SETUP:MODE? ->  
:SEARCH1:SPIBUS:SETUP:MODE WIRE3

### **:SEARCh<x>:TRACe<x>:LEVel**

**Function** Sets the threshold level of the trace or queries the current setting.

**Syntax** :SEARCh<x>:TRACe<x>:LEVel  
{<NRf>|<Voltage>|<Current>}  
:SEARCh<x>:TRACe<x>:LEVel?  
<x> of SEARCh<x> = 1 or 2  
<x> of TRACe<x> = 1 to 8  
<NRf>, <Voltage>, and <Current> = See the *User's Manual (IM701310-01E)*.

**Example** :SEARCH1:TRACE1:LEVEL 0  
:SEARCH1:TRACE1:LEVEL? ->  
:SEARCH1:TRACE1:LEVEL 0.000E+00

**Description** This command applies to the channel corresponding to the source specified by the following commands.

- :SEARCh<x>:I2CBus:CLOCK:SOURce
- :SEARCh<x>:STRace
- :SEARCh<x>:SPIBus:CLOCK:SOURce
- :SEARCh<x>:SPIBus:CS:TRACe
- :SEARCh<x>:SPIBus:DATA[1-2]:TRACe

### **:SEARCh<x>:TYPE**

**Function** Sets the search type or queries the current setting.

**Syntax** :SEARCh<x>:TYPE {CANBus|EDGE|EQUAlify|  
I2CBus|SPATtern|SPIBus|STATe|WIDTh}  
:SEARCh<x>:TYPE?  
<x> = 1 or 2

**Example** :SEARCH1:TYPE CANBus  
:SEARCH1:TYPE? -> :SEARCH1:TYPE CANBus

## 4.5 TRIGger Group

### **:TRIGger:EINterval:EVENT<x>:CANBus?**

**Function** Queries all settings related to the CAN bus trigger of the event.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:  
ACK DONTCARE;BRATE 1000000;DATA:  
BORDER BIG;CONDITION DONTCARE;  
DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "111001010110010001111000100100  
110010101000100001000111111111010";  
SIGNUNSIGN;:TRIGGER:EINTERVAL:EVENT1:  
CANBUS:IDEXT:PATTERN "XXXXXXXXXXXXXXXXXX  
XXXXXXXXXXXX";:TRIGGER:EINTERVAL:  
EVENT1:CANBUS:IDOR:ID1:ACK DONTCARE;  
DATA:BORDER BIG;CONDITION DONTCARE;  
DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "000000010010001101000101011001  
1110001001101010111100110111101111";  
SIGN UNSIGN;:TRIGGER:EINTERVAL:EVENT1:  
CANBUS:IDOR:ID1:FORMAT STD;IDEXT:  
PATTERN "11010101111001101111011110000";:  
TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDSTD:PATTERN "00100100011";:  
TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:MODE 0;RTR DATA;:TRIGGER:EINTERVAL:  
EVENT1:CANBUS:IDOR:ID2:ACK DONTCARE;  
DATA:BORDER BIG;CONDITION DONTCARE;  
DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "11111101101110010111010100110  
000110110010101000011001000010000";  
SIGN UNSIGN;:TRIGGER:EINTERVAL:EVENT1:  
CANBUS:IDOR:ID2:FORMAT STD;IDEXT:  
PATTERN "10010001101000101011001111000";:  
TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID2:IDSTD:PATTERN "10001010110";:  
TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID2:MODE 0.....

### **:TRIGger:EINterval:EVENT<x>:CANBus:ACK**

**Function** Sets the ACK condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
ACK {ACK|ACKBoth|DONTcare|NONack}  
:TRIGger:EINterval:EVENT<x>:CANBus:ACK?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
ACK ACK  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:  
ACK? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:  
ACK ACK

### **:TRIGger:EINterval:EVENT<x>:CANBus:**

#### **BRATe**

**Function** Sets the bit rate (data transfer rate) of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
BRATe {<Nrf>|USER,<Nrf>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
BRATe?  
<x> = 1, 2  
<Nrf> = 83300, 125000, 250000, 500000, 1000000  
<Nrf> of USER = See the *User's Manual*  
(IM701310-01E).

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
BRATE 83300  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:  
BRATE? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:  
BRATE 83300

### **:TRIGger:EINterval:EVENT<x>:CANBus:**

#### **DATA?**

**Function** Queries all settings related to the CAN bus signal trigger data.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
DATA? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
BORDER BIG;CONDITION DONTCARE;  
DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "111001010110010001111000100100  
110010101000100001000111111111010";  
SIGN UNSIGN

## 4.5 TRIGger Group

### **:TRIGger:EINterval:EVENT<x>:CANBus: DATA:BORder**

Function Sets the byte order of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:BORder {BIG|LITtle}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:BORder?  
<x> = 1, 2

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
BORDER BIG  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
BORDER? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
BORDER BIG

### **:TRIGger:EINterval:EVENT<x>:CANBus: DATA:CONDition**

Function Sets the data condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:CONDition {BETween|DONTcare|FALSE|  
GTHan|LTHan|ORANge|TRUE}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:CONDition?  
<x> = 1, 2

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
CONDITION BETWEEN  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
CONDITION? ->  
TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
CONDITION BETWEEN

### **:TRIGger:EINterval:EVENT<x>:CANBus: DATA:DATA<x>**

Function Sets the comparison data of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:DATA<x> {<NRf>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:DATA<x>?  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2

<NRf> = See the *User's Manual (IM701310-01E)*.

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
DATA:DATA1 1  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
DATA1? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
DATA1 1.0000000E+00

Description

- Use :TRIGger:EINterval:EVENT<x>:CANBus:DATA:DATA1 when :TRIGger:EINterval:EVENT<x>:CANBus:DATA:CONDition GTHan is specified.  
Use :TRIGger:EINterval:EVENT<x>:CANBus:DATA:DATA2 when :TRIGger:EINterval:EVENT<x>:CANBus:DATA:CONDition LTHan is specified.
- Use :TRIGger:EINterval:EVENT<x>:CANBus:DATA:DATA1 to set the smaller value and :TRIGger:EINterval:EVENT<x>:CANBus:DATA:DATA2 to set the larger value when :TRIGger:EINterval:EVENT<x>:CANBus:DATA:CONDition BETWEEN|ORANge is specified.

### **:TRIGger:EINterval:EVENT<x>:CANBus: DATA:DLC**

Function Sets the number of valid bytes (DLC) of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:DLC {<NRf>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:DLC?  
<x> = 1, 2  
<NRf> = 0 to 8

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
DLC 0  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
DLC? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
DLC 0

**:TRIGger:EINterval:EVENT<x>:CANBus:****DATA:HEXA**

Function Sets the CAN bus signal trigger data in hexadecimal notation.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:HEXA {<String>}  
<x> = 1, 2  
<String> = Up to 16 characters by combining '0' to 'F' and 'X' (in one-byte unit)

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
DATA:HEXA "A9"

**:TRIGger:EINterval:EVENT<x>:CANBus:****DATA:MSBLsb**

Function Sets the MSB and LSB bits of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:MSBLsb {<Nrf>,<Nrf>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:MSBLsb?  
<x> = 1, 2  
<Nrf> = See the *User's Manual (IM701310-01E)*.

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
MSBLSB 1,0  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
MSBLSB? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
MSBLSB 1,0

**:TRIGger:EINterval:EVENT<x>:CANBus:****DATA:PATtern**

Function Sets the CAN bus signal trigger data in binary notation or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:PATtern {<String>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:PATtern?  
<x> = 1, 2  
<String> = Up to 64 characters by combining '0','1,' and 'X' (in one-byte unit)

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
PATTERN "11011111"  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
PATTERN "11011111"

**:TRIGger:EINterval:EVENT<x>:CANBus:****DATA:SIGN**

Function Sets the sign of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:SIGN {SIGN|UNSign}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
DATA:SIGN?  
<x> = 1, 2

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
SIGN SIGN  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
SIGN? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:DATA:  
SIGN SIGN

**:TRIGger:EINterval:EVENT<x>:CANBus:****IDEXt?**

Function Queries all settings related to the ID of the extended format of the CAN bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDEXt?  
<x> = 1, 2

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
IDEXt? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDEXt:  
PATTERN "1100101101110000111011101111"

**:TRIGger:EINterval:EVENT<x>:CANBus:****IDEXt:HEXA**

Function Sets the ID of the extended format of the CAN bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDEXt:  
HEXA {<String>}  
<x> = 1, 2  
<String> = 8 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDEXt:  
HEXA "1AEF5906"

## 4.5 TRIGger Group

### **:TRIGger:EINterval:EVENT<x>:CANBus:IDEXt:PATtern**

**Function** Sets the ID of the extended format of the CAN bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:IDEXt:PATtern {<String>}  
:TRIGger:EINterval:EVENT<x>:CANBus:IDEXt:PATtern?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDEXT:PATTERN "11001011011100001110111011111"  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDEXT:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDEXT:PATTERN "11001011011100001110111011111"

### **:TRIGger:EINterval:EVENT<x>:CANBus:IDOR?**

**Function** Queries all settings related to the OR condition of the CAN bus signal trigger.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:IDOR?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:ACK DONTCARE;DATA:BORDER BIG;CONDITION DONTCARE;DATA1 0.0000000E+00;DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;PATTERN "00000001001000110100010101100111100010010101111001101010111100110111101111";SIGN UNSIGN;:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:FORMAT STD;IDEXT:PATTERN "110101011100110111011110000";:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:IDSTD:PATTERN "00100100011";:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:MODE 0;RTR DATA;:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID2:ACK DONTCARE;DATA:BORDER BIG;CONDITION DONTCARE;DATA1 0.0000000E+00;DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;PATTERN "111111011011100101110101001100110100010000";SIGN UNSIGN;:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID2:FORMAT STD;IDEXT:PATTERN"10010001101000101011001111000";:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID2:IDSTD:PATTERN "10001010110";:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID2:MODE 0;RTR DATA;:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID3:ACK DONTCARE;DATA:BORDER BIG;CONDITION DONTCARE;DATA1 0.0000000E+00;DATA2 255.00000E+00;DLC 8.....

### **:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>?**

**Function** Queries all settings related to each ID of the OR condition of the CAN bus signal trigger.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:ACK DONTCARE;DATA:BORDER BIG;CONDITION DONTCARE;DATA1 0.0000000E+00;DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;PATTERN "0000000100100011010001010110111100010010101011110011011100110111101111";SIGN UNSIGN;:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:FORMAT STD;IDEXT:PATTERN "1101010111001101110111011110000";:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:IDSTD:PATTERN"00100100011";:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:MODE 0;RTR DATA

### **:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:ACK**

**Function** Sets each ACK condition of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:ACK {ACK|ACKBoth|DONTcare|NONack}  
:TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:ACK?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:ACK ACK  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:ACK? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:ID1:ACK ACK



**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA?**

**Function** Queries all settings related to each data of the OR condition of the CAN bus signal trigger.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:BORDER BIG;CONDITION DONTCARE;  
DATA1 0.0000000E+00;  
DATA2 255.000000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "000000010010001101000101011001  
11100010011010111100110111101111";  
SIGN UNSIGN

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:BORDER**

**Function** Sets byte order of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:BORDER {BIG|LITTLE}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:BORDER?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:BORDER BIG  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:BORDER? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:BORDER BIG

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:CONDition**

**Function** Sets each data condition of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:CONDition {BETween|  
DONTcare|FALSE|GTHan|LTHan|ORANge|TRUE}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:CONDition?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:CONDITION BETWEEN  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:CONDITION? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:CONDITION BETWEEN

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:DATA<x>**

**Function** Sets comparison data of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:DATA<x> {<NRf>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:DATA<x>?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<x> of DATA<x> = 1 or 2  
<NRf> = See the *User's Manual (IM701310-01E)*.

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:DATA1 1  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:DATA1? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:DATA1 1.0000000E+00

**Description**

- Use :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:DATA1 when :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:CONDition GTHan is specified.
- Use :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:DATA2 when :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:CONDition LTHan is specified.
- Use :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:DATA1 to set the smaller value and :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:DATA2 to set the larger value when :TRIGger:EINterval:EVENT<x>:CANBus:IDOR:ID<x>:DATA:CONDition BETween|ORANge is specified.

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:DLC**

**Function** Sets the number of valid bytes (DLC) of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:DLC {<NRf>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:DLC?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<NRf> = 0 to 8

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:DLC 0  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:DLC? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:DLC 0

## 4.5 TRIGger Group

### **:TRIGger:EINTerval:EVENT<x>:CANBus:**

#### **IDOR:ID<x>:DATA:HEXA**

**Function** Sets each data of the OR condition of the CAN bus signal trigger in hexadecimal notation.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:HEXA {<String>}  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<String> = Up to 16 characters by combining '0' to 'F' and 'X' (in one-byte unit)

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:HEXA "A9"

### **:TRIGger:EINTerval:EVENT<x>:CANBus:**

#### **IDOR:ID<x>:DATA:MSBLSb**

**Function** Sets the MSB and LSB bits of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:MSBLSb {<Nrf>,<Nrf>}  
:TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:MSBLSb?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<Nrf> = See the *User's Manual (IM701310-01E)*.

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:MSBLSB 1,0  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:MSBLSB? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:MSBLSB 1,0

### **:TRIGger:EINTerval:EVENT<x>:CANBus:**

#### **IDOR:ID<x>:DATA:PATtern**

**Function** Sets each data of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:PATtern {<String>}  
:TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:PATtern?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<String> = Up to 64 characters by combining '0','1,' and 'X' (in one-byte unit)

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:PATTERN "11011111"  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:PATTERN "11011111"

### **:TRIGger:EINTerval:EVENT<x>:CANBus:**

#### **IDOR:ID<x>:DATA:SIGN**

**Function** Sets sign of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:SIGN {SIGN|UNSign}  
:TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:DATA:SIGN?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:SIGN SIGN  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:SIGN? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:DATA:SIGN SIGN

### **:TRIGger:EINTerval:EVENT<x>:CANBus:**

#### **IDOR:ID<x>:FORMat**

**Function** Sets each message format (standard or extended) of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:FORMat {STD|EXT}  
:TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:FORMat?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:FORMAT STD  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:FORMAT? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:FORMAT STD

### **:TRIGger:EINTerval:EVENT<x>:CANBus:**

#### **IDOR:ID<x>:IDEXt?**

**Function** Queries all settings related to the ID of each extended format of the OR condition of the CAN bus signal trigger.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDEXt?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDEXT? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDEXT:PATTERN "1100101101110000111  
0111011111"

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDEXt:HEXA**

Function Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDEXt:HEXA {<String>}  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<String> = 8 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDEXT:HEXA "1AEF5906"

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDEXt:PATtern**

Function Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDEXt:PATtern {<String>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDEXt:PATtern?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<String> = 29 characters by combining '0', '1,' and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDEXT:PATTERN "11001011011100001110  
111011111"  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDEXT:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDEXT:PATTERN "11001011011100001110  
111011111"

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDSTd?**

Function Queries all settings related to the ID of each standard format of the OR condition of the CAN bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDSTd?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
IDOR:ID1:IDSTD? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDSTD:PATTERN "00011111101"

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDSTd:HEXA**

Function Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDSTd:HEXA {<String>}  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<String> = 3 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDSTD:HEXA "5DF"

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDSTd:PATtern**

Function Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDSTd:PATtern {<String>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:IDSTd:PATtern?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4  
<String> = 11 characters by combining '0', '1,' and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDSTD:PATTERN "10111011111"  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDSTD:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:IDSTD:PATTERN "10111011111"

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:MODE**

Function Enables or disables each condition of the OR condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:MODE {<Boolean>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:MODE?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:MODE ON  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:MODE? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:MODE 1

**:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:RTR**

Function Sets each RTR of the OR condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:RTR {DATA|DONTcare|REMOte}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
IDOR:ID<x>:RTR?  
<x> of EVENT<x> = 1 or 2  
<x> of ID<x> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:RTR DATA  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:RTR? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDOR:  
ID1:RTR DATA

## 4.5 TRIGger Group

### **:TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd?**

**Function** Queries all settings related to the ID of the standard format of the CAN bus signal trigger.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDSTd? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDSTd:  
PATTERN "00011111101"

### **:TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd:HEXA**

**Function** Sets the ID of the standard format of the CAN bus signal trigger in hexadecimal notation.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd:HEXA {<String>}  
<x> = 1, 2  
<String> = 8 characters by combining '0' to 'F' and 'X'

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDSTd:HEXA "5DF"

### **:TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd:PATtern**

**Function** Sets the ID of the standard format of the CAN bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd:PATtern {<String>}  
:TRIGger:EINTerval:EVENT<x>:CANBus:IDSTd:PATtern?  
<x> = 1, 2  
<String> = 11 characters by combining '0','1,' and 'X'

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:IDSTd:PATtern "10111011111"  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDSTd:PATtern? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:IDSTd:PATtern "10111011111"

### **:TRIGger:EINTerval:EVENT<x>:CANBus:MODE**

**Function** Sets the CAN bus signal trigger mode or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:MODE {EFrame|IDExt|IDOR|IDSTd|SOF}  
:TRIGger:EINTerval:EVENT<x>:CANBus:MODE?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:MODE EFRAME  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:MODE? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:MODE EFRAME

### **:TRIGger:EINTerval:EVENT<x>:CANBus:REcessive**

**Function** Sets the recessive level (bus level) of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:REcessive {HIGH|LOW}  
:TRIGger:EINTerval:EVENT<x>:CANBus:REcessive?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:RECESSIVE HIGH  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:RECESSIVE? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:RECESSIVE HIGH

### **:TRIGger:EINTerval:EVENT<x>:CANBus:RTR**

**Function** Sets the RTR of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:RTR {DATA|DONTcare|REMOte}  
:TRIGger:EINTerval:EVENT<x>:CANBus:RTR?  
<x> = 1, 2

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:RTR DATA  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:RTR? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:RTR DATA

### **:TRIGger:EINTerval:EVENT<x>:CANBus:SOURCE**

**Function** Sets the trigger source of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:CANBus:SOURCE {<NRf>}  
:TRIGger:EINTerval:EVENT<x>:CANBus:SOURCE?  
<x> = 1, 2  
<NRf> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:CANBUS:SOURCE 1  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:SOURCE? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:SOURCE 1

**:TRIGger:EINterval:EVENT<x>:CANBus:SPOint**

Function Sets the sample point of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:CANBus:  
SPOint {<Nrf>}  
:TRIGger:EINterval:EVENT<x>:CANBus:  
SPOint?  
<x> = 1, 2  
<Nrf> = 18.8 to 90.6(%)

Example :TRIGGER:EINTERVAL:EVENT1:CANBUS:  
SPOINT 18.8  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:  
SPOINT? ->  
:TRIGGER:EINTERVAL:EVENT1:CANBUS:  
SPOINT 18.8E+00

**:TRIGger:EINterval:EVENT<x>:I2Cbus?**

Function Queries all settings related to the I<sup>2</sup>C bus signal trigger of the event.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN "1011101111";  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110";  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS:PATTERN "10101011";  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7APSUB:SADDRESS:PATTERN "10101011";  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
TYPE BIT10ADDRESS;:TRIGGER:EINTERVAL:  
EVENT1:I2CBUS:CLOCK:SOURCE 1;:TRIGGER:  
EINTERVAL:EVENT1:I2CBUS:DATA:BYTE 1;  
CONDITION TRUE;DPOSITION 1;MODE 1;  
PATTERN1 "10101011";  
PATTERN2 "10101010";  
PATTERN3 "10101111";  
PATTERN4 "10101011";PMODE DONTCARE;  
SOURCE 1;:TRIGGER:EINTERVAL:EVENT1:  
I2CBUS:GCALL:BIT7MADDRESS:  
PATTERN "1010101";:TRIGGER:EINTERVAL:  
EVENT1:I2CBUS:GCALL:  
SBYTE BIT7MADDRESS;:TRIGGER:EINTERVAL:  
EVENT1:I2CBUS:MODE ADATA;NAIGNORE:  
HSMODE 1;RACCESS 1;SBYTE 1;:TRIGGER:  
EINTERVAL:EVENT1:I2CBUS:SBHSMODE:  
TYPE HSMODE

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATA?**

Function Queries all settings related to the address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
ADATA?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA?  
-> :TRIGGER:EINTERVAL:EVENT1:I2CBUS:  
ADATA:BIT10ADDRESS:  
PATTERN "1011101111";:TRIGGER:  
EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS:  
PATTERN "11011110";:TRIGGER:EINTERVAL:  
EVENT1:I2CBUS:ADATA:BIT7APSUB:ADDRESS:  
PATTERN "10101011";:TRIGGER:EINTERVAL:  
EVENT1:I2CBUS:ADATA:BIT7APSUB:SADDRESS:  
PATTERN "10101011";:TRIGGER:EINTERVAL:  
EVENT1:I2CBUS:ADATA:TYPE BIT10ADDRESS

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATA:BIT10address?**

Function Queries all settings related to the 10-bit address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
ADATA:BIT10address?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT10ADDRESS? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN "1011101111"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATA:BIT10address:HEXA**

Function Sets the 10-bit address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
ADATA:BIT10address:HEXA {<String>}  
<x> = 1 or 2

<String> = 3 characters by combining '0' to 'F' and 'X' (bit 8 is the R/W bit)

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT10ADDRESS:HEXA "7AB"

## 4.5 TRIGger Group

### **:TRIGger:EINTerval:EVENT<x>:I2Cbus:**

#### **ADATa:BIT10address:PATtern**

Function Sets the 10-bit address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT10address:PATtern {<String>}  
:TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT10address:PATtern?  
<x> = 1 or 2

<String> = 11 characters by combining '0', '1', and 'X' (bit 8 is the R/W bit)

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN "1011101111"  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN "1011101111"

### **:TRIGger:EINTerval:EVENT<x>:I2Cbus:**

#### **ADATa:BIT7Address?**

Function Queries all settings related to the 7-bit address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT7Address?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110"

### **:TRIGger:EINTerval:EVENT<x>:I2Cbus:**

#### **ADATa:BIT7Address:HEXA**

Function Sets the 7-bit address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT7Address:HEXA {<String>}  
<x> = 1 or 2  
<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is the R/W bit)

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS:HEXA "DE"

### **:TRIGger:EINTerval:EVENT<x>:I2Cbus:**

#### **ADATa:BIT7Address:PATtern**

Function Sets the 7-bit address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT7Address:PATtern {<String>}  
:TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT7Address:PATtern?  
<x> = 1 or 2

<String> = 8 characters by combining '0', '1', and 'X' (bit 0 is the R/W bit)

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110"  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110"

### **:TRIGger:EINTerval:EVENT<x>:I2Cbus:**

#### **ADATa:BIT7APsub?**

Function Queries all settings related to the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT7APsub?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7APSUB? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS:PATTERN "10101011";:  
TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7APSUB:SADDRESS:PATTERN "10101011"

### **:TRIGger:EINTerval:EVENT<x>:I2Cbus:**

#### **ADATa:BIT7APsub:ADDRESS?**

Function Queries all settings related to the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINTerval:EVENT<x>:I2Cbus:  
ADATa:BIT7APsub:ADDRESS?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS:PATTERN "10101011"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:ADDRESS:HEXA**

**Function** Sets the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

**Syntax** :TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:ADDRESS:HEXA {<String>}  
<x> = 1 or 2  
<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is the R/W bit)

**Example** :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:ADDRESS:HEXA "AB"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:ADDRESS:PATtern**

**Function** Sets the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:ADDRESS:PATtern {<String>}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:ADDRESS:PATtern?  
<x> = 1 or 2  
<String> = 8 characters by combining '0', '1', and 'X' (bit 0 is the R/W bit)

**Example** :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:ADDRESS:PATTERN "10101011"  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:ADDRESS:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:ADDRESS:PATTERN "10101011"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:SADdress?**

**Function** Queries all settings related to the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger.

**Syntax** :TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:SADdress?  
<x> = 1 or 2

**Example** :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:SADDRESS? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:SADDRESS:PATTERN "10101011"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:SADdress:HEXA**

**Function** Sets the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

**Syntax** :TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:SADdress:HEXA {<String>}  
<x> = 1 or 2  
<String> = 2 characters by combining '0' to 'F' and 'X'

**Example** :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:SADDRESS:HEXA "EF"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:SADdress:PATtern**

**Function** Sets the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:SADdress:PATtern {<String>}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:BIT7APsub:SADdress:PATtern?  
<x> = 1 or 2  
<String> = 8 characters by combining '0', '1', and 'X'

**Example** :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:SADDRESS:PATTERN "10101011"  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:SADDRESS:PATTERN? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:BIT7APSUB:SADDRESS:PATTERN "10101011"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:TYPE**

**Function** Sets the address type of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:TYPE {BIT10address|BIT7Address|BIT7APsub}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:ADATa:TYPE?  
<x> = 1 or 2

**Example** :TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:TYPE BIT10ADDRESS  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:TYPE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:ADATA:TYPE BIT10ADDRESS

**:TRIGger:EINterval:EVENT<x>:I2Cbus:CLOCK?**

**Function** Queries all settings related to the clock channel of the I<sup>2</sup>C bus signal trigger.

**Syntax** :TRIGger:EINterval:EVENT<x>:I2Cbus:CLOCK?  
<x> = 1 or 2

**Example** :TRIGGER:EINTERVAL:EVENT1:I2CBUS:CLOCK? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:CLOCK:SOURCE 1

## 4.5 TRIGger Group

### **:TRIGger:EINTerval:EVENT<x>:I2CBus: CLOCK:SOURCE**

Function Sets the clock channel of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:I2CBus:  
CLOCK:SOURCE {<Nrf>}  
:TRIGger:EINTerval:EVENT<x>:I2CBus:  
CLOCK:SOURCE?  
<x> = 1 or 2  
<Nrf> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:CLOCK:  
SOURCE 1  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:CLOCK:  
SOURCE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:CLOCK:  
SOURCE 1

### **:TRIGger:EINTerval:EVENT<x>:I2CBus: DATA?**

Function Queries all settings related to the data of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:  
DATA? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
BYTE 1;CONDITION TRUE;DPOSITION 1;  
MODE 1;PATTERN1 "10101011";  
PATTERN2 "10101010";  
PATTERN3 "10101111";  
PATTERN4 "10101011";PMODE DONTCARE;  
SOURCE 1

### **:TRIGger:EINTerval:EVENT<x>:I2CBus: DATA:BYTE**

Function Sets the number of data bytes of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA:BYTE {<Nrf>}  
:TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA:BYTE?  
<x> = 1 or 2  
<Nrf> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
BYTE 1  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
BYTE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
BYTE 1

### **:TRIGger:EINTerval:EVENT<x>:I2CBus: DATA:CONDITION**

Function Sets the determination method (match or not match) of the data of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA:CONDITION {FALSE|TRUE}  
:TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA:CONDITION?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
CONDITION TRUE  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
CONDITION? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
CONDITION TRUE

### **:TRIGger:EINTerval:EVENT<x>:I2CBus: DATA:DPOSITION**

Function Sets the position for comparing the data pattern of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA:DPOSITION {<Nrf>}  
:TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA:DPOSITION?  
<x> = 1 or 2  
<Nrf> = 0 to 9999

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
DPOSITION 1  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
DPOSITION? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
DPOSITION 1

### **:TRIGger:EINTerval:EVENT<x>:I2CBus: DATA:HEXA<x>**

Function Sets the data of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINTerval:EVENT<x>:I2CBus:  
DATA:HEXA<x> {<String>}  
<x> of EVENT<x> = 1 or 2  
<x> of HEXA<x> = 1 to 4  
<String> = 2 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
HEXA1 "AB"



**:TRIGger:EINterval:EVENT<x>:I2Cbus:****DATA:MODE**

Function Enables/Disables the data conditions of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:MODE {<Boolean>}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:MODE?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
MODE ON  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
MODE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
MODE 1

**:TRIGger:EINterval:EVENT<x>:I2Cbus:****DATA:PATtern<x>**

Function Sets the data of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:PATtern<x> {<String>}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:PATtern<x>?  
<x> of EVENT<x> = 1 or 2  
<x> of <PATtern x> = 1 to 4  
<String> = 8 characters by combining '0', '1', and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
PATTERN1 "10101011"  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
PATTERN1? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
PATTERN1 "10101011"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:****DATA:PMODE**

Function Sets the pattern comparison start position mode of the data of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:PMODE {DONTcare|SELEct}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:PMODE?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
PMODE SELECT  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
PMODE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
PMODE SELECT

**:TRIGger:EINterval:EVENT<x>:I2Cbus:****DATA:SOURce**

Function Sets the data channel of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:SOURce {<NRf>}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:  
DATA:SOURce?  
<x> = 1 or 2  
<NRf> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
SOURCE 1  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
SOURCE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:DATA:  
SOURCE 1

**:TRIGger:EINterval:EVENT<x>:I2Cbus:****GCALl?**

Function Queries all settings related to the general call of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
GCALl?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:  
GCALL? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:GCALL:  
BIT7MADDRESS:PATTERN "10101011";  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:GCALL:  
SBYTE BIT7MADDRESS

**:TRIGger:EINterval:EVENT<x>:I2Cbus:****GCALl:BIT7maddress?**

Function Queries all settings related to the 7-bit master address of the general call of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
GCALl:BIT7maddress?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:GCALL:  
BIT7MADDRESS? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:GCALL:  
BIT7MADDRESS:PATTERN "10101011"

**:TRIGger:EINterval:EVENT<x>:I2Cbus:****GCALl:BIT7maddress:HEXA**

Function Sets the 7-bit master address of the general call of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:  
GCALl:BIT7maddress:HEXA {<String>}  
<x> = 1 or 2

<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is fixed to 1)

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:GCALL:  
BIT7MADDRESS:HEXA "AB"

## 4.5 TRIGGER Group

### **:TRIGGER:EVENT<x>:I2CBUS:**

#### **GCALL:BIT7maddress:PATtern**

**Function** Sets the 7-bit master address of the general call of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGGER:EVENT<x>:I2CBUS:  
GCALL:BIT7maddress:PATtern {<String>}  
:TRIGGER:EVENT<x>:I2CBUS:  
GCALL:BIT7maddress:PATtern?  
<x> = 1 or 2  
<String> = 7 characters by combining '0', '1', and 'X'

**Example** :TRIGGER:EVENT1:I2CBUS:  
GCALL:BIT7MADDRESS:PATTERN "1010101"  
:TRIGGER:EVENT1:I2CBUS:GCALL:  
BIT7MADDRESS:PATTERN? ->  
:TRIGGER:EVENT1:I2CBUS:GCALL:  
BIT7MADDRESS:PATTERN "1010101"

### **:TRIGGER:EVENT<x>:I2CBUS:**

#### **GCALL:SBYTE (Second Byte)**

**Function** Sets the second byte type of the general call of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGGER:EVENT<x>:I2CBUS:  
GCALL:SBYTE {BIT7maddress|DONTcare|H04|  
H06}  
:TRIGGER:EVENT<x>:I2CBUS:  
GCALL:SBYTE?  
<x> = 1 or 2

**Example** :TRIGGER:EVENT1:I2CBUS:GCALL:  
SBYTE BIT7MADDRESS  
:TRIGGER:EVENT1:I2CBUS:GCALL:  
SBYTE? ->  
:TRIGGER:EVENT1:I2CBUS:GCALL:  
SBYTE BIT7MADDRESS

### **:TRIGGER:EVENT<x>:**

#### **I2CBUS:MODE**

**Function** Sets the trigger mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGGER:EVENT<x>:I2CBUS:  
MODE {ADATA|ESTart|GCALL|NAIgnore|  
SBHSmode}  
:TRIGGER:EVENT<x>:I2CBUS:  
MODE?  
<x> = 1 or 2

**Example** :TRIGGER:EVENT1:I2CBUS:  
MODE ADATA  
:TRIGGER:EVENT1:I2CBUS:  
MODE? ->  
:TRIGGER:EVENT1:I2CBUS:  
MODE ADATA

### **:TRIGGER:EVENT<x>:I2CBUS:**

#### **NAIgnore?**

**Function** Queries all settings related to the NON ACK ignore mode of the I<sup>2</sup>C bus signal trigger.

**Syntax** :TRIGGER:EVENT<x>:I2CBUS:  
NAIgnore?  
<x> = 1 or 2

**Example** :TRIGGER:EVENT1:I2CBUS:  
NAIGNORE? ->  
:TRIGGER:EVENT1:I2CBUS:  
NAIGNORE:HSMODE 1;RACCESS 1;SBYTE 1

### **:TRIGGER:EVENT<x>:I2CBUS:**

#### **NAIgnore:HSMODE**

**Function** Sets whether to ignore NON ACK in high speed mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGGER:EVENT<x>:I2CBUS:  
NAIgnore:HSMODE {<Boolean>}  
:TRIGGER:EVENT<x>:I2CBUS:  
NAIgnore:HSMODE?  
<x> = 1 or 2

**Example** :TRIGGER:EVENT1:I2CBUS:  
NAIGNORE:HSMODE ON  
:TRIGGER:EVENT1:I2CBUS:  
NAIGNORE:HSMODE? ->  
:TRIGGER:EVENT1:I2CBUS:  
NAIGNORE:HSMODE 1

### **:TRIGGER:EVENT<x>:I2CBUS:**

#### **NAIgnore:RACcess**

**Function** Sets whether to ignore NON ACK in read access mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGGER:EVENT<x>:I2CBUS:  
NAIgnore:RACcess {<Boolean>}  
:TRIGGER:EVENT<x>:I2CBUS:  
NAIgnore:RACcess?  
<x> = 1 or 2

**Example** :TRIGGER:EVENT1:I2CBUS:  
NAIGNORE:RACCESS ON  
:TRIGGER:EVENT1:I2CBUS:  
NAIGNORE:RACCESS? ->  
:TRIGGER:EVENT1:I2CBUS:  
NAIGNORE:RACCESS 1

**:TRIGger:EINterval:EVENT<x>:I2Cbus:NAIgnore:SBYTE (Start Byte)**

Function Sets whether to ignore NON ACK in the start byte of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:NAIgnore:SBYTE {<Boolean>}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:NAIgnore:SBYTE?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:NAIGNORE:SBYTE ON  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:NAIGNORE:SBYTE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:NAIGNORE:SBYTE 1

**:TRIGger:EINterval:EVENT<x>:I2Cbus:SBHSMODE?**

Function Queries all settings related to the start byte and high speed mode of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:SBHSMODE?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:SBHSMODE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:SBHSMODE:TYPE HSMODE

**:TRIGger:EINterval:EVENT<x>:I2Cbus:SBHSMODE:TYPE**

Function Sets the type of the start byte or high speed mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:I2Cbus:SBHSMODE:TYPE {HSMODE|SBYTE}  
:TRIGger:EINterval:EVENT<x>:I2Cbus:SBHSMODE:TYPE?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:I2CBUS:SBHSMODE:TYPE HSMODE  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:SBHSMODE:TYPE? ->  
:TRIGGER:EINTERVAL:EVENT1:I2CBUS:SBHSMODE:TYPE HSMODE

**:TRIGger:EINterval:EVENT<x>:SPIBUS?**

Function Queries all settings related to the SPI bus signal trigger of the event.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBUS?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:BITORDER LSBFIRST;CLOCK:POLARITY FALL;SOURCE 1;:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:ACTIVE HIGH;SOURCE 1;:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:BYTE 1;CONDITION TRUE;DPOSITION 1;PATTERN1 "00010010";PATTERN2 "00110100";PATTERN3 "01010110";PATTERN4 "00010010";SOURCE 3;:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA2:BYTE 4;CONDITION TRUE;DPOSITION 1;PATTERN1 "00010010";PATTERN2 "00110100";PATTERN3 "01010110";PATTERN4 "00010010";SOURCE 3;:TRIGGER:EINTERVAL:EVENT1:SPIBUS:MODE WIRE3

**:TRIGger:EINterval:EVENT<x>:SPIBUS:BITORDER**

Function Sets the bit order of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBUS:BITORDER {LSBFirst|MSBFirst}  
:TRIGger:EINterval:EVENT<x>:SPIBUS:BITORDER?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:BITORDER LSBFIRST  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:BITORDER? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:BITORDER LSBFIRST

**:TRIGger:EINterval:EVENT<x>:SPIBUS:CLOCK?**

Function Queries all settings related to the clock channel of the SPI bus signal trigger.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBUS:CLOCK?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK:POLARITY FALL;SOURCE 1

## 4.5 TRIGger Group

### **:TRIGger:EINTerval:EVENT<x>:SPIBus: CLOCK:POLarity**

Function Sets the polarity of the clock channel of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:SPIBus:  
CLOCK:POLarity {FALL|RISE}  
:TRIGger:EINTerval:EVENT<x>:SPIBus:  
CLOCK:POLarity?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK:  
POLARITY FALL  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK:  
POLARITY? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK:  
POLARITY FALL

### **:TRIGger:EINTerval:EVENT<x>:SPIBus: CLOCK:SOURce**

Function Sets the clock channel of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:SPIBus:  
CLOCK:SOURce {<Nrf>}  
:TRIGger:EINTerval:EVENT<x>:SPIBus:  
CLOCK:SOURce?  
<x> = 1 or 2  
<Nrf> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK:  
SOURCE 1  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK:  
SOURCE? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CLOCK:  
SOURCE 1

### **:TRIGger:EINTerval:EVENT<x>: SPIBus:CS?**

Function Queries all settings related to the chip select channel of the SPI bus signal trigger.

Syntax :TRIGger:EINTerval:EVENT<x>:SPIBus:CS?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:  
ACTIVE HIGH;SOURCE 1

### **:TRIGger:EINTerval:EVENT<x>:SPIBus: CS:ACTive**

Function Sets the active level of the chip select channel of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:SPIBus:CS:  
ACTive {HIGH|LOW}  
:TRIGger:EINTerval:EVENT<x>:SPIBus:CS:  
ACTive?  
<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:  
ACTIVE HIGH  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:  
ACTIVE? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:  
ACTIVE HIGH

### **:TRIGger:EINTerval:EVENT<x>:SPIBus: CS:SOURce**

Function Sets the chip select channel of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINTerval:EVENT<x>:SPIBus:CS:  
SOURce {<Nrf>}  
:TRIGger:EINTerval:EVENT<x>:SPIBus:CS:  
SOURce?  
<x> = 1 or 2  
<Nrf> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:  
SOURCE 1  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:  
SOURCE? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:CS:  
SOURCE 1

### **:TRIGger:EINTerval:EVENT<x>:SPIBus: DATA<x>?**

Function Queries all settings related to the data of the SPI bus signal trigger.

Syntax :TRIGger:EINTerval:EVENT<x>:SPIBus:  
DATA<x>?  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:  
DATA1? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:  
BYTE 1;CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "00010010";SOURCE 3

Description DATA2 is valid when :TRIGger:EINTerval:  
EVENT<x>:SPIBus:MODE WIRE4 is specified.

**:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:BYTE**

Function Sets the number of bytes of the data of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:BYTE {<Nrf>}  
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:BYTE?  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<Nrf> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:BYTE 1  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:BYTE? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:BYTE 1

**:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:CONDition**

Function Sets the determination method (match or not match) of the data of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:CONDition {FALSE|TRUE}  
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:CONDition?  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:CONDITION TRUE  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:CONDITION? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:CONDITION TRUE

**:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:DPOSition**

Function Sets the pattern comparison start position of the data of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:DPOSition {<Nrf>}  
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:DPOSition?  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<Nrf> = 0 to 9999

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:DPOSITION 1  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:DPOSITION? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:DPOSITION 1

**:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:HEXA<x>**

Function Sets the data of the SPI bus signal trigger in hexadecimal notation.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:HEXA<x> {<String>}  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<x> of HEXA<x> = 1 to 4  
<String> = 2 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:HEXA1 "AB"

**:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:PATtern<x>**

Function Sets the data of the SPI bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:PATtern<x> {<String>}  
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:PATtern<x>?  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<x> of <PATtern x> = 1 to 4  
<String> = 8 characters by combining '0', '1', and 'X'

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:PATTERN1 "10101011"  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:PATTERN1? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:PATTERN1 "10101011"

**:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:SOURce**

Function Sets the trace of the data of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:SOURce {<Nrf>}  
:TRIGger:EINterval:EVENT<x>:SPIBus:DATA<x>:SOURce?  
<x> of EVENT<x> = 1 or 2  
<x> of DATA<x> = 1 or 2  
<Nrf> = 1 to 4

Example :TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:SOURCE 1  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:SOURCE? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:DATA1:SOURCE 1

## 4.5 TRIGger Group

### **:TRIGger:EINTerval:EVENT<x>:SPIBus:**

#### **MODE**

**Function** Sets the wiring system of the SPI bus signal trigger (three-wire or four-wire) or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:SPIBus:  
MODE {WIRE3|WIRE4}  
:TRIGger:EINTerval:EVENT<x>:SPIBus:  
MODE?  
<x> = 1 or 2

**Example** :TRIGGER:EINTERVAL:EVENT1:SPIBUS:  
MODE WIRE3  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:  
MODE? ->  
:TRIGGER:EINTERVAL:EVENT1:SPIBUS:  
MODE WIRE3

### **:TRIGger:EINTerval:EVENT<x>:STATE: CHANnel<x>**

**Function** Sets the condition to be satisfied of the channel or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:STATE:  
CHANnel<x> {DONTcare|HIGH|LOW}  
:TRIGger:EINTerval:EVENT<x>:STATE:  
CHANnel<x>?  
<x> of EVENT<x> = 1 or 2  
<x> of CHANnel<x> = 1 to 4

**Example** :TRIGGER:EINTERVAL:EVENT1:STATE:  
CHANNEL1 HIGH  
:TRIGGER:EINTERVAL:EVENT1:STATE:  
CHANNEL1? ->  
:TRIGGER:EINTERVAL:EVENT1:STATE:  
CHANNEL1 HIGH

**Description** This command is valid when :TRIGger:  
EINTerval:EVENT<x>:TYPE I2CBus.

### **:TRIGger:EINTerval:EVENT<x>:TYPE**

**Function** Sets the trigger type of the event or queries the current setting.

**Syntax** :TRIGger:EINTerval:EVENT<x>:  
TYPE {CANBus|EDGE|EQUalify|I2CBus|  
PQUalify|PSTATE|PULSE|SPATtern|SPIBus|  
STATE}  
:TRIGger:EINTerval:EVENT<x>:TYPE?  
<x> = 1 or 2

**Example** :TRIGGER:EINTERVAL:EVENT1:TYPE CANBUS  
:TRIGGER:EINTERVAL:EVENT1:TYPE? ->  
:TRIGGER:EINTERVAL:EVENT1:TYPE CANBUS

### **:TRIGger:ENHanced:CANBus?**

**Function** Queries all settings related to the CAN bus signal trigger.

**Syntax** :TRIGger:ENHanced:CANBus?

**Example** :TRIGGER:ENHANCED:CANBUS? ->  
:TRIGGER:ENHANCED:CANBUS:ACK DONTCARE;  
BRATE 1000000;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.000000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "111001010110010001111000100100  
110010101000100001000111111111010";  
SIGN UNSIGN;:TRIGGER:ENHANCED:CANBUS:  
IDEXT:PATTERN "XXXXXXXXXXXXXXXXXXXXXX  
XXXXX";:TRIGGER:ENHANCED:CANBUS:IDOR:  
ID1:ACK DONTCARE;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.000000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "000000010010001101000101011001  
1110001001101010111100110111101111";  
SIGN UNSIGN;:TRIGGER:ENHANCED:CANBUS:  
IDOR:ID1:FORMAT STD;IDEXT:  
PATTERN "11010101111001101111011110000";:  
TRIGGER:ENHANCED:CANBUS:IDOR:ID1:IDSTD:  
PATTERN "00100100011";:TRIGGER:  
ENHANCED:CANBUS:IDOR:ID1:MODE 0;  
RTR DATA;:TRIGGER:ENHANCED:CANBUS:IDOR:  
ID2:ACK DONTCARE;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.000000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "111111101101110010111010100110  
0001110110010101000011001000010000";  
SIGN UNSIGN;:TRIGGER:ENHANCED:CANBUS:  
IDOR:ID2:FORMAT STD;IDEXT:  
PATTERN "10010001101000101011001111000";:  
TRIGGER:ENHANCED:CANBUS:IDOR:ID2:IDSTD:  
PATTERN "10001010110";:TRIGGER:  
ENHANCED:CANBUS:IDOR:ID2:MODE 0.....

### **:TRIGger:ENHanced:CANBus:ACK**

**Function** Sets the ACK condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:  
ACK {ACK|ACKBoth|DONTcare|NONack}  
:TRIGger:ENHanced:CANBus:ACK?

**Example** :TRIGGER:ENHANCED:CANBUS:ACK ACK  
:TRIGGER:ENHANCED:CANBUS:ACK? ->  
:TRIGGER:ENHANCED:CANBUS:ACK ACK

**:TRIGger:ENHanced:CANBus:BRATe**

Function Sets the bit rate (data transfer rate) of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:BRATe {<Nrf>|USER,<Nrf>}  
:TRIGger:ENHanced:CANBus:BRATe?<Nrf> = 83300, 125000, 250000, 500000, 1000000<Nrf> of USER = See the *User's Manual (IM701310-01E)*.

Example :TRIGGER:ENHANCED:CANBUS:BRATE 83300  
:TRIGGER:ENHANCED:CANBUS:BRATE? ->  
:TRIGGER:ENHANCED:CANBUS:BRATE 83300

**:TRIGger:ENHanced:CANBus:DATA?**

Function Queries all settings related to the CAN bus signal trigger data.

Syntax :TRIGger:ENHanced:CANBus:DATA?  
Example :TRIGGER:ENHANCED:CANBUS:DATA? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:  
BORDER BIG;CONDITION DONTCARE;  
DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "11100101011001000111100010010010011001010001000010001111111111010";  
SIGN UNSIGN

**:TRIGger:ENHanced:CANBus:DATA:BORDER**

Function Sets the byte order of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:DATA:BORDER {BIG|LITTLE}  
:TRIGger:ENHanced:CANBus:DATA:BORDER?

Example :TRIGGER:ENHANCED:CANBUS:DATA:  
BORDER BIG  
:TRIGGER:ENHANCED:CANBUS:DATA:  
BORDER? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:  
BORDER BIG

**:TRIGger:ENHanced:CANBus:DATA:CONDition**

Function Sets the data condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:DATA:CONDition {BETWEEen|DONTcare|FALSE|GTHan|LTHan|ORANge|TRUE}  
:TRIGger:ENHanced:CANBus:DATA:CONDition?

Example :TRIGGER:ENHANCED:CANBUS:DATA:  
CONDITION BETWEEN  
:TRIGGER:ENHANCED:CANBUS:DATA:  
CONDITION? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:  
CONDITION BETWEEN

**:TRIGger:ENHanced:CANBus:DATA:DATA<x>**

Function Sets the comparison data of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:DATA:DATA<x> {<Nrf>}  
:TRIGger:ENHanced:CANBus:DATA:DATA<x>?<x> = 1, 2  
<Nrf> = See the *User's Manual (IM701310-01E)*.

Example :TRIGGER:ENHANCED:CANBUS:DATA:DATA1 1  
:TRIGGER:ENHANCED:CANBUS:DATA:DATA1? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:  
DATA1 1.0000000E+00

Description • Use :TRIGger:ENHANCED:CANBus:DATA:DATA1 when :TRIGger:ENHANCED:CANBus:DATA:CONDition GTHan is specified.  
• Use :TRIGger:ENHANCED:CANBus:DATA:DATA2 when :TRIGger:ENHANCED:CANBus:DATA:CONDition LTHan is specified.  
• Use :TRIGger:ENHANCED:CANBus:DATA:DATA1 to set the smaller value and :TRIGger:ENHANCED:CANBus:DATA:DATA2 to set the larger value when :TRIGger:ENHANCED:CANBus:DATA:CONDition BETWEEen|ORANge is specified.

**:TRIGger:ENHanced:CANBus:DATA:DLC**

Function Sets the number of valid bytes (DLC) of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:DATA:DLC {<Nrf>}  
:TRIGger:ENHanced:CANBus:DATA:DLC?<Nrf> = 0 to 8

Example :TRIGGER:ENHANCED:CANBUS:DATA:DLC 0  
:TRIGGER:ENHANCED:CANBUS:DATA:DLC? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:DLC 0

**:TRIGger:ENHanced:CANBus:DATA:HEXA**

Function Sets the CAN bus signal trigger data in hexadecimal notation.

Syntax :TRIGger:ENHanced:CANBus:DATA:HEXA {<String>}  
<String> = Up to 16 characters by combining '0' to 'F' and 'X' (in one-byte unit)

Example :TRIGGER:ENHANCED:CANBUS:DATA:HEXA "A9"

## 4.5 TRIGger Group

### **:TRIGger:ENHanced:CANBus:DATA:MSBLSb**

Function Sets the MSB and LSB bits of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:DATA:MSBLSb {<Nrf>,<Nrf>}  
:TRIGger:ENHanced:CANBus:DATA:MSBLSb? <Nrf> = See the *User's Manual (IM701310-01E)*.

Example :TRIGGER:ENHANCED:CANBUS:DATA:MSBLSB 1,0  
:TRIGGER:ENHANCED:CANBUS:DATA:MSBLSB? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:MSBLSB 1,0

### **:TRIGger:ENHanced:CANBus:DATA:PATtern**

Function Sets the CAN bus signal trigger data in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:DATA:PATtern {<String>}  
:TRIGger:ENHanced:CANBus:DATA:PATtern? <String> = Up to 64 characters by combining '0','1,' and 'X' (in one-byte unit)

Example :TRIGGER:ENHANCED:CANBUS:DATA:PATTERN "11011111"  
:TRIGGER:ENHANCED:CANBUS:DATA:PATTERN? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:PATTERN "11011111"

### **:TRIGger:ENHanced:CANBus:DATA:SIGN**

Function Sets the sign of the CAN bus signal trigger data or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:DATA:SIGN {SIGN|UNSign}  
:TRIGger:ENHanced:CANBus:DATA:SIGN?

Example :TRIGGER:ENHANCED:CANBUS:DATA:SIGN SIGN  
:TRIGGER:ENHANCED:CANBUS:DATA:SIGN? ->  
:TRIGGER:ENHANCED:CANBUS:DATA:SIGN SIGN

### **:TRIGger:ENHanced:CANBus:IDEXt?**

Function Queries all settings related to the ID of the extended format of the CAN bus signal trigger.

Syntax :TRIGger:ENHanced:CANBus:IDEXt?

Example :TRIGGER:ENHANCED:CANBUS:IDEXT? ->  
:TRIGGER:ENHANCED:CANBUS:IDEXT:  
PATTERN "11001011011100001110111011111"

### **:TRIGger:ENHanced:CANBus:IDEXt:HEXA**

Function Sets the ID of the extended format of the CAN bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:CANBus:IDEXt:HEXA {<String>}  
<String> = 8 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:ENHANCED:CANBUS:IDEXT:HEXA "1AEF5906"

### **:TRIGger:ENHanced:CANBus:IDEXt:PATtern**

Function Sets the ID of the extended format of the CAN bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:IDEXt:PATtern {<String>}  
:TRIGger:ENHanced:CANBus:IDEXt:PATtern? <String> = 29 characters by combining '0','1,' and 'X'

Example :TRIGGER:ENHANCED:CANBUS:IDEXT:PATTERN "11001011011100001110111011111"  
:TRIGGER:ENHANCED:CANBUS:IDEXT:PATTERN? ->  
:TRIGGER:ENHANCED:CANBUS:IDEXT:PATTERN "11001011011100001110111011111"

### **:TRIGger:ENHanced:CANBus:IDOR?**

Function Queries all settings related to the OR condition of the CAN bus signal trigger.

Syntax :TRIGger:ENHanced:CANBus:IDOR?

Example :TRIGGER:ENHANCED:CANBUS:IDOR? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
ACK DONTCARE;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "000000010010001101000101011001110001001101010111100110111011111";  
SIGN UNSIGN;;TRIGGER:ENHANCED:CANBUS:IDOR:ID1:FORMAT STD;IDEXT:  
PATTERN "11010101111001101111011110000";  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:IDSTD:  
PATTERN "00100100011";:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:MODE 0;  
RTR DATA;;TRIGGER:ENHANCED:CANBUS:IDOR:ID2:ACK DONTCARE;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "111111011011100101110101001100011011001010100011001000010000";  
SIGN UNSIGN;;TRIGGER:ENHANCED:CANBUS:IDOR:ID2:FORMAT STD;IDEXT:  
PATTERN "10010001101000101011001111000";  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID2:IDSTD:  
PATTERN "10001010110";:TRIGGER:ENHANCED:CANBUS:IDOR:ID2:MODE 0;  
RTR DATA;;TRIGGER:ENHANCED:CANBUS:IDOR:ID3:ACK DONTCARE;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.0000000E+00;  
DATA2 255.00000E+00;DLC 8.....



**:TRIGger:ENHanced:CANBus:IDOR:ID<x>?**

Function Queries all settings related to each ID of the OR condition of the CAN bus signal trigger.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
ACK DONTCARE;DATA:BORDER BIG;  
CONDITION DONTCARE;DATA1 0.000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB  
7,0;PATTERN "00000001001000110100010101  
10011110001001101010111100110111101111";  
SIGN UNSIGN;:TRIGGER:ENHANCED:CANBUS:  
IDOR:ID1:FORMAT STD;IDEXT:  
PATTERN "11010101111001101111011110000";:  
TRIGGER:ENHANCED:CANBUS:IDOR:ID1:IDSTD:  
PATTERN "00100100011";:TRIGGER:  
ENHANCED:CANBUS:IDOR:ID1:MODE 0;  
RTR DATA

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****ACK**

Function Sets each ACK condition of the OR condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
ACK {ACK|ACKBoth|DONTcare|NONack}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
ACK?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
ACK ACK  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
ACK? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
ACK ACK

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****DATA?**

Function Queries all settings related to each data of the OR condition of the CAN bus signal trigger.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
DATA? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
BORDER BIG;CONDITION DONTCARE;  
DATA1 0.000000E+00;  
DATA2 255.00000E+00;DLC 8;MSBLSB 7,0;  
PATTERN "000000010010001101000101011001  
1110001001101010111100110111101111";  
SIGN UNSIGN

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****DATA:BORDER**

Function Sets byte order of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:BORDER {BIG|LITTLE}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:BORDER?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
BORDER BIG  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
BORDER? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
BORDER BIG

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****DATA:CONDition**

Function Sets each data condition of the OR condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:CONDition {BETween|DONTcare|FALSE|  
GTHan|LTHan|ORANGE|TRUE}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:CONDition?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
CONDITION BETWEEN  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
CONDITION? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
CONDITION BETWEEN

## 4.5 TRIGger Group

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>:**

#### **DATA:DATA<x>**

**Function** Sets comparison data of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:DATA<x> {<NRf>}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:DATA<x>?  
<x> of ID<x> = 1 to 4  
<x> of DATA<x> = 1 or 2  
<NRf> = See the *User's Manual (IM701310-01E)*.

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
DATA1 1  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
DATA1? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
DATA1 1.0000000E+00

**Description**

- Use :TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:DATA1 when :TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:CONDITION GTHan is specified.
- Use :TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:DATA2 when :TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:CONDITION LTHan is specified.
- Use :TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:DATA1 to set the smaller value and :TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:DATA2 to set the larger value when :TRIGger:ENHanced:CANBus:IDOR:ID<x>:DATA:CONDITION BETWEEN|ORANGE is specified.

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>:**

#### **DATA:DLC**

**Function** Sets the number of valid bytes (DLC) of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:DLC {<NRf>}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:DLC?  
<x> = 1 to 4  
<NRf> = 0 to 8

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
DLC 0  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
DLC? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
DLC 0

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>:**

#### **DATA:HEXA**

**Function** Sets each data of the OR condition of the CAN bus signal trigger in hexadecimal notation.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:HEXA {<String>}  
<x> = 1 to 4  
<String> = Up to 16 characters by combining '0' to 'F' and 'X' (in one-byte unit)

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
HEXA "A9"

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>:**

#### **DATA:MSBLSb**

**Function** Sets the MSB and LSB bits of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:MSBLSb {<NRf>,<NRf>}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:MSBLSb?  
<x> = 1 to 4  
<NRf> = See the *User's Manual (IM701310-01E)*.

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
MSBLSB 1,0  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
MSBLSB? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
MSBLSB 1,0

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>:**

#### **DATA:PATtern**

**Function** Sets each data of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:PATtern {<String>}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:PATtern?  
<x> = 1 to 4  
<String> = Up to 64 characters by combining '0', '1', and 'X' (in one-byte unit)

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
PATTERN "11011111"  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
PATTERN? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
PATTERN "11011111"

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****DATA:SIGN**

Function Sets sign of each data of the OR condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:SIGN {SIGN|UNSign}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
DATA:SIGN?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
SIGN SIGN  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
SIGN? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:DATA:  
SIGN SIGN

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****FORMat**

Function Sets each message format (standard or extended) of the OR condition of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
FORMat {STD|EXT}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
FORMat?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
FORMAT STD  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
FORMAT? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
FORMAT STD

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****IDEXt?**

Function Queries all settings related to the ID of each extended format of the OR condition of the CAN bus signal trigger.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDEXt?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDEXT? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDEXT:PATTERN "110010110111000011101110  
11111"

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****IDEXt:HEXA**

Function Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDEXt:HEXA {<String>}  
<x> = 1 to 4  
<String> = 8 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDEXT:HEXA "1AEF5906"

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****IDEXt:PATtern**

Function Sets the ID of each extended format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDEXt:PATtern {<String>}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDEXt:PATtern?  
<x> = 1 to 4  
<String> = 29 characters by combining '0', '1', and 'X'

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDEXT:PATTERN "110010110111000011101110  
11111"  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDEXT:PATTERN? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDEXT:PATTERN "110010110111000011101110  
11111"

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****IDSTd?**

Function Queries all settings related to the ID of each standard format of the OR condition of the CAN bus signal trigger.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDSTd?  
<x> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDSTD? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDSTD:PATTERN "00011111101"

**:TRIGger:ENHanced:CANBus:IDOR:ID<x>:****IDSTd:HEXA**

Function Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDSTd:HEXA {<String>}  
<x> = 1 to 4  
<String> = 3 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDSTD:HEXA "5DF"

## 4.5 TRIGger Group

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>: IDSTd:PATtern**

**Function** Sets the ID of each standard format of the OR condition of the CAN bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDSTd:PATtern {<String>}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
IDSTd:PATtern?  
<x> = 1 to 4  
<String> = 11 characters by combining '0','1,' and 'X'

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDSTD:PATTERN "10111011111"  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDSTD:PATTERN? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
IDSTD:PATTERN "10111011111"

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>: MODE**

**Function** Enables or disables each condition of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
MODE {<Boolean>}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
MODE?  
<x> = 1 to 4

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
MODE ON  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
MODE? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
MODE 1

### **:TRIGger:ENHanced:CANBus:IDOR:ID<x>: RTR**

**Function** Sets each RTR of the OR condition of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
RTR {DATA|DONTcare|REMOte}  
:TRIGger:ENHanced:CANBus:IDOR:ID<x>:  
RTR?  
<x> = 1 to 4

**Example** :TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
RTR DATA  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
RTR? ->  
:TRIGGER:ENHANCED:CANBUS:IDOR:ID1:  
RTR DATA

### **:TRIGger:ENHanced:CANBus:IDSTd?**

**Function** Queries all settings related to the ID of the standard format of the CAN bus signal trigger.

**Syntax** :TRIGger:ENHanced:CANBus:IDSTd?

**Example** :TRIGGER:ENHANCED:CANBUS:IDSTD? ->  
:TRIGGER:ENHANCED:CANBUS:IDSTD:  
PATTERN "00011111101"

### **:TRIGger:ENHanced:CANBus:IDSTd:HEXA**

**Function** Sets the ID of the standard format of the CAN bus signal trigger in hexadecimal notation.

**Syntax** :TRIGger:ENHanced:CANBus:IDSTd:  
HEXA {<String>}  
<String> = 3 characters by combining '0' to 'F' and 'X'

**Example** :TRIGGER:ENHANCED:CANBUS:IDSTD:  
HEXA "5DF"

### **:TRIGger:ENHanced:CANBus:IDSTd:PATtern**

**Function** Sets the ID of the standard format of the CAN bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:IDSTd:  
PATtern {<String>}  
:TRIGger:ENHanced:CANBus:IDSTd:PATtern?  
<String> = 11 characters by combining '0','1,' and 'X'

**Example** :TRIGGER:ENHANCED:CANBUS:IDSTD:  
PATTERN "10111011111"  
:TRIGGER:ENHANCED:CANBUS:IDSTD:  
PATTERN? ->  
:TRIGGER:ENHANCED:CANBUS:IDSTD:  
PATTERN "10111011111"

### **:TRIGger:ENHanced:CANBus:MODE**

**Function** Sets the CAN bus signal trigger mode or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:  
MODE {EFrame|IDExt|IDOR|IDSTd|SOF}  
:TRIGger:ENHanced:CANBus:MODE?

**Example** :TRIGGER:ENHANCED:CANBUS:MODE EFRAME  
:TRIGGER:ENHANCED:CANBUS:MODE? ->  
:TRIGGER:ENHANCED:CANBUS:MODE EFRAME

### **:TRIGger:ENHanced:CANBus:REcessive**

**Function** Sets the recessive level (bus level) of the CAN bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:CANBus:  
REcessive {HIGH|LOW}  
:TRIGger:ENHanced:CANBus:REcessive?

**Example** :TRIGGER:ENHANCED:CANBUS:RECESSIVE HIGH  
:TRIGGER:ENHANCED:CANBUS:RECESSIVE? ->  
:TRIGGER:ENHANCED:CANBUS:RECESSIVE HIGH

**:TRIGger:ENHanced:CANBus:RTR**

Function Sets the RTR of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:  
RTR {DATA|DONTcare|REMOte}  
:TRIGger:ENHanced:CANBus:RTR?

Example :TRIGGER:ENHANCED:CANBUS:RTR DATA  
:TRIGGER:ENHANCED:CANBUS:RTR? ->  
:TRIGGER:ENHANCED:CANBUS:RTR DATA

**:TRIGger:ENHanced:CANBus:SOURce**

Function Sets the trigger source of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:SOURce {<NRf>}  
:TRIGger:ENHanced:CANBus:SOURce?  
<NRf> = 1 to 4

Example :TRIGGER:ENHANCED:CANBUS:SOURCE 1  
:TRIGGER:ENHANCED:CANBUS:SOURCE? ->  
:TRIGGER:ENHANCED:CANBUS:SOURCE 1

**:TRIGger:ENHanced:CANBus:SPOint**

Function Sets the sample point of the CAN bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:CANBus:SPOint {<NRf>}  
:TRIGger:ENHanced:CANBus:SPOint?  
<NRf> = 18.8 to 90.6(%)

Example :TRIGGER:ENHANCED:CANBUS:SPOINT 18.8  
:TRIGGER:ENHANCED:CANBUS:SPOINT? ->  
:TRIGGER:ENHANCED:CANBUS:  
SPOINT 18.8E+00

**:TRIGger:ENHanced:I2CBus?**

Function Queries all settings related to the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2CBus?  
Example :TRIGGER:ENHANCED:I2CBUS? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN "1011101111";:  
TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110";:  
TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS:PATTERN "10101011";:  
TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB:SADDRESS:PATTERN "10101011";:  
TRIGGER:ENHANCED:I2CBUS:ADATA:  
TYPE BIT10ADDRESS;:TRIGGER:ENHANCED:  
I2CBUS:CLOCK:SOURCE 1;:TRIGGER:  
ENHANCED:I2CBUS:DATA:BYTE 1;  
CONDITION TRUE;DPOSITION 1;MODE 1;  
PATTERN1 "10101011";  
PATTERN2 "10101010";  
PATTERN3 "10101111";  
PATTERN4 "10101011";PMODE DONTCARE;  
SOURCE 1;:TRIGGER:ENHANCED:I2CBUS:  
GCALL:BIT7MADDRESS:PATTERN "1010101";:  
TRIGGER:ENHANCED:I2CBUS:GCALL:  
SBYTE BIT7MADDRESS;:TRIGGER:ENHANCED:  
I2CBUS:MODE ADATA;NAIGNORE:HSMODE 1;  
RACCESS 1;SBYTE 1;:TRIGGER:ENHANCED:  
I2CBUS:SBHSMODE:TYPE HSMODE

**:TRIGger:ENHanced:I2CBus:ADATa?**

Function Queries all settings related to the address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2CBus:ADATa?

Example :TRIGGER:ENHANCED:I2CBUS:ADATa? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT10ADDRESS:PATTERN "1011101111";:  
TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7ADDRESS:PATTERN "11011110";:  
TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:ADDRESS:PATTERN "10101011";:  
TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:SADDRESS:PATTERN "10101011";:  
TRIGGER:ENHANCED:I2CBUS:ADATa:  
TYPE BIT10ADDRESS

**:TRIGger:ENHanced:I2CBus:ADATa:****BIT10address?**

Function Queries all settings related to the 10-bit address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT10address?

Example :TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT10ADDRESS? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT10ADDRESS:PATTERN "1011101111"

## 4.5 TRIGger Group

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT10address:HEXA**

Function Sets the 10-bit address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT10address:HEXA {<String>}  
<String> = 3 characters by combining '0' to 'F' and 'X' (bit 8 is the R/W bit)

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT10ADDRESS:HEXA "7AB"

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT10address:PATtern**

Function Sets the 10-bit address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT10address:PATtern {<String>}  
:TRIGger:ENHanced:I2CBus:ADATa:  
BIT10address:PATtern?  
<String> = 11 characters by combining '0', '1', and 'X' (bit 8 is the R/W bit)

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN "10111011111"  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT10ADDRESS:PATTERN "10111011111"

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT7Address?**

Function Queries all settings related to the 7-bit address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT7Address?

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7ADDRESS? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110"

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT7Address:HEXA**

Function Sets the 7-bit address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT7Address:HEXA {<String>}  
<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is the R/W bit)

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7ADDRESS:HEXA "DE"

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT7Address:PATtern**

Function Sets the 7-bit address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT7Address:PATtern {<String>}  
:TRIGger:ENHanced:I2CBus:ADATa:  
BIT7Address:PATtern?  
<String> = 8 characters by combining '0', '1', and 'X' (bit 0 is the R/W bit)

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110"  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7ADDRESS:PATTERN "11011110"

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT7APsub?**

Function Queries all settings related to the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT7APsub?

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS:PATTERN "10101011";:  
TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB:SADDRESS:PATTERN "10101011"

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT7APsub:ADDRess?**

Function Queries all settings related to the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT7APsub:ADDRess?

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS:PATTERN "10101011"

### **:TRIGger:ENHanced:I2CBus:ADATa:**

#### **BIT7APsub:ADDRess:HEXA**

Function Sets the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:I2CBus:ADATa:  
BIT7APsub:ADDRess:HEXA {<String>}  
<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is the R/W bit)

Example :TRIGGER:ENHANCED:I2CBUS:ADATA:  
BIT7APSUB:ADDRESS:HEXA "AB"

**:TRIGger:ENHanced:I2Cbus:ADATa:****BIT7APsub:ADDRESS:PATtern**

Function Sets the 7-bit address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:ADATa:  
BIT7APsub:ADDRESS:PATtern {<String>}  
:TRIGger:ENHanced:I2Cbus:ADATa:  
BIT7APsub:ADDRESS:PATtern?  
<String> = 8 characters by combining '0', '1', and 'X'  
(bit 0 is the R/W bit)

Example :TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:ADDRESS:PATTERN "10101011"  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:ADDRESS:PATTERN? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:ADDRESS:PATTERN "10101011"

**:TRIGger:ENHanced:I2Cbus:ADATa:****BIT7APsub:SADDRESS?**

Function Queries all settings related to the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2Cbus:ADATa:  
BIT7APsub:SADDRESS?

Example :TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:SADDRESS? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:SADDRESS:PATTERN "10101011"

**:TRIGger:ENHanced:I2Cbus:ADATa:****BIT7APsub:SADDRESS:HEXA**

Function Sets the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:I2Cbus:ADATa:  
BIT7APsub:SADDRESS:HEXA {<String>}  
<String> = 2 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:SADDRESS:HEXA "EF"

**:TRIGger:ENHanced:I2Cbus:ADATa:****BIT7APsub:SADDRESS:PATtern**

Function Sets the Sub address of the 7-bit + Sub address of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:ADATa:  
BIT7APsub:SADDRESS:PATtern {<String>}  
:TRIGger:ENHanced:I2Cbus:ADATa:  
BIT7APsub:SADDRESS:PATtern?  
<String> = 8 characters by combining '0', '1', and 'X'

Example :TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:SADDRESS:PATTERN "10101011"  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:SADDRESS:PATTERN? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
BIT7APSUB:SADDRESS:PATTERN "10101011"

**:TRIGger:ENHanced:I2Cbus:ADATa:TYPE**

Function Sets the address type of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:ADATa:  
TYPE {BIT10address|BIT7Address|  
BIT7APsub}  
:TRIGger:ENHanced:I2Cbus:ADATa:TYPE?

Example :TRIGGER:ENHANCED:I2CBUS:ADATa:  
TYPE BIT10ADDRESS  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
TYPE? ->  
:TRIGGER:ENHANCED:I2CBUS:ADATa:  
TYPE BIT10ADDRESS

**:TRIGger:ENHanced:I2Cbus:CLOCK?**

Function Queries all settings related to the clock channel of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2Cbus:CLOCK?

Example :TRIGGER:ENHANCED:I2CBUS:CLOCK? ->  
:TRIGGER:ENHANCED:I2CBUS:CLOCK:SOURCE 1

**:TRIGger:ENHanced:I2Cbus:CLOCK:****SOURCE**

Function Sets the clock channel of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:CLOCK:  
SOURCE {<NRF>}  
:TRIGger:ENHanced:I2Cbus:CLOCK:SOURCE?  
<NRF> = 1 to 4

Example :TRIGGER:ENHANCED:I2CBUS:CLOCK:SOURCE 1  
:TRIGGER:ENHANCED:I2CBUS:CLOCK:  
SOURCE? ->  
:TRIGGER:ENHANCED:I2CBUS:CLOCK:  
SOURCE 1

**:TRIGger:ENHanced:I2Cbus:DATA?**

Function Queries all settings related to the data of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2Cbus:DATA?  
<x> = 1 or 2

Example :TRIGGER:ENHANCED:I2CBUS:DATA? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:BYTE 1;  
CONDITION TRUE;DPOSITION 1;MODE 1;  
PATTERN1 "10101011";  
PATTERN2 "10101010";  
PATTERN3 "10101111";  
PATTERN4 "10101011";PMODE DONTCARE;  
SOURCE 1

## 4.5 TRIGger Group

### **:TRIGger:ENHanced:I2CBus:DATA:BYTE**

Function Sets the number of data bytes of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
BYTE {<NRf>}  
:TRIGger:ENHanced:I2CBus:DATA:BYTE?  
<NRf> = 1 to 4

Example :TRIGGER:ENHANCED:I2CBUS:DATA:BYTE 1  
:TRIGGER:ENHANCED:I2CBUS:DATA:BYTE? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:BYTE 1

### **:TRIGger:ENHanced:I2CBus:DATA:**

#### **CONDition**

Function Sets the determination method (match or not match) of the data of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
CONDition {FALSE|TRUE}  
:TRIGger:ENHanced:I2CBus:DATA:  
CONDition?

Example :TRIGGER:ENHANCED:I2CBUS:DATA:  
CONDITION TRUE  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
CONDITION? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
CONDITION TRUE

### **:TRIGger:ENHanced:I2CBus:DATA:**

#### **DPOSITION**

Function Sets the position for comparing the data pattern of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
DPOSITION {<NRf>}  
:TRIGger:ENHanced:I2CBus:DATA:  
DPOSITION?  
<NRf> = 0 to 9999

Example :TRIGGER:ENHANCED:I2CBUS:DATA:  
DPOSITION 1  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
DPOSITION? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
DPOSITION 1

### **:TRIGger:ENHanced:I2CBus:DATA:**

#### **HEXA<x>**

Function Sets the data of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
HEXA<x> {<String>}  
<x> = 1 to 4  
<String> = 2 characters by combining '0' to 'F' and 'X'

Example :TRIGGER:ENHANCED:I2CBUS:DATA:  
HEXA1 "AB"

### **:TRIGger:ENHanced:I2CBus:DATA:MODE**

Function Enables/Disables the data conditions of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
MODE {<Boolean>}  
:TRIGger:ENHanced:I2CBus:DATA:MODE?

Example :TRIGGER:ENHANCED:I2CBUS:DATA:MODE ON  
:TRIGGER:ENHANCED:I2CBUS:DATA:MODE? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:MODE 1

### **:TRIGger:ENHanced:I2CBus:DATA:**

#### **PATtern<x>**

Function Sets the data of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
PATtern<x> {<String>}  
:TRIGger:ENHanced:I2CBus:DATA:  
PATtern<x>?  
<x> = 1 to 4  
<String> = 8 characters by combining '0', '1', and 'X'

Example :TRIGGER:ENHANCED:I2CBUS:DATA:  
PATTERN1 "10101011"  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
PATTERN1? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
PATTERN1 "10101011"

### **:TRIGger:ENHanced:I2CBus:DATA:PMODE**

Function Sets the pattern comparison start position mode of the data of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
PMODE {DONTcare|SELECT}  
:TRIGger:ENHanced:I2CBus:DATA:PMODE?

Example :TRIGGER:ENHANCED:I2CBUS:DATA:  
PMODE SELECT  
:TRIGGER:ENHANCED:I2CBUS:DATA:PMODE? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
PMODE SELECT

### **:TRIGger:ENHanced:I2CBus:DATA:SOURce**

Function Sets the data trace of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2CBus:DATA:  
SOURce {<NRf>}  
:TRIGger:ENHanced:I2CBus:DATA:  
SOURce?  
<NRf> = 1 to 4

Example :TRIGGER:ENHANCED:I2CBUS:DATA:SOURCE 1  
:TRIGGER:ENHANCED:I2CBUS:DATA:  
SOURCE? ->  
:TRIGGER:ENHANCED:I2CBUS:DATA:SOURCE 1



**:TRIGger:ENHanced:I2Cbus:GCALl?**

Function Queries all settings related to the general call of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2Cbus:GCALl?  
<x> = 1 or 2

Example :TRIGGER:ENHANCED:I2CBUS:GCALL? ->  
:TRIGGER:ENHANCED:I2CBUS:GCALL:  
BIT7ADDRESS:PATTERN "1010101";  
TRIGGER:ENHANCED:I2CBUS:GCALL:  
SBYTE BIT7ADDRESS

**:TRIGger:ENHanced:I2Cbus:GCALl:BIT7address?**

Function Queries all settings related to the 7-bit master address of the general call of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2Cbus:GCALl:  
BIT7address?  
<x> = 1 or 2

Example :TRIGGER:ENHANCED:I2CBUS:GCALL:  
BIT7ADDRESS? ->  
:TRIGGER:ENHANCED:I2CBUS:GCALL:  
BIT7ADDRESS:PATTERN "1010101"

**:TRIGger:ENHanced:I2Cbus:GCALl:BIT7address:HEXA**

Function Sets the 7-bit master address of the general call of the I<sup>2</sup>C bus signal trigger in hexadecimal notation.

Syntax :TRIGger:ENHanced:I2Cbus:GCALl:  
BIT7address:HEXA {<String>}  
<x> = 1 or 2  
<String> = 2 characters by combining '0' to 'F' and 'X' (bit 0 is fixed to '1')

Example :TRIGGER:ENHANCED:I2CBUS:GCALL:  
BIT7ADDRESS:HEXA "AB"

**:TRIGger:ENHanced:I2Cbus:GCALl:BIT7address:PATtern**

Function Sets the 7-bit master address of the general call of the I<sup>2</sup>C bus signal trigger in binary notation or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:GCALl:  
BIT7address:PATtern {<String>}  
:TRIGger:ENHanced:I2Cbus:GCALl:  
BIT7address:PATtern?  
<x> = 1 or 2  
<String> = 7 characters by combining '0', '1', and 'X'

Example :TRIGGER:ENHANCED:I2CBUS:GCALL:  
BIT7ADDRESS:PATTERN "1010101"  
:TRIGGER:ENHANCED:I2CBUS:GCALL:  
BIT7ADDRESS:PATTERN? ->  
:TRIGGER:ENHANCED:I2CBUS:GCALL:  
BIT7ADDRESS:PATTERN "1010101"

**:TRIGger:ENHanced:I2Cbus:GCALl:SBYTE (Second Byte)**

Function Sets the second byte type of the general call of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:GCALl:  
SBYTE {BIT7address|DONTcare|H04|H06}  
:TRIGger:ENHanced:I2Cbus:GCALl:SBYTE?

Example :TRIGGER:ENHANCED:I2CBUS:GCALL:  
SBYTE BIT7ADDRESS  
:TRIGGER:ENHANCED:I2CBUS:GCALL:  
SBYTE? ->  
:TRIGGER:ENHANCED:I2CBUS:GCALL:  
SBYTE BIT7ADDRESS

**:TRIGger:ENHanced:I2Cbus:MODE**

Function Sets the trigger mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:  
MODE {ADATa|ESTart|GCALl|NAIGnore|  
SBHSmode}  
:TRIGger:ENHanced:I2Cbus:MODE?

Example :TRIGGER:ENHANCED:I2CBUS:MODE ADATA  
:TRIGGER:ENHANCED:I2CBUS:MODE? ->  
:TRIGGER:ENHANCED:I2CBUS:MODE ADATA

**:TRIGger:ENHanced:I2Cbus:NAIGnore?**

Function Queries all settings related to the NON ACK ignore mode of the I<sup>2</sup>C bus signal trigger.

Syntax :TRIGger:ENHanced:I2Cbus:NAIGnore?  
Example :TRIGGER:ENHANCED:I2CBUS:NAIGNORE? ->  
:TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
HSMODE 1;RACCESS 1;SBYTE 1

**:TRIGger:ENHanced:I2Cbus:NAIGnore:HSMode**

Function Sets whether to ignore NON ACK in high speed mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:I2Cbus:NAIGnore:  
HSMode {<Boolean>}  
:TRIGger:ENHanced:I2Cbus:NAIGnore:  
HSMode?

Example :TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
HSMODE ON  
:TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
HSMODE? ->  
:TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
HSMODE 1

## 4.5 TRIGger Group

### **:TRIGger:ENHanced:I2CBus:NAIGnore: RACcEss**

**Function** Sets whether to ignore NON ACK in read access mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:I2CBus:NAIGnore:  
RACcEss {<Boolean>}  
:TRIGger:ENHanced:I2CBus:NAIGnore:  
RACcEss?

**Example** :TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
RACCESS ON  
:TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
RACCESS? ->  
:TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
RACCESS 1

### **:TRIGger:ENHanced:I2CBus:NAIGnore: SBYte (Start Byte)**

**Function** Sets whether to ignore NON ACK in the start byte of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:I2CBus:NAIGnore:  
SBYte {<Boolean>}  
:TRIGger:ENHanced:I2CBus:NAIGnore:  
SBYte?

**Example** :TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
SBYTE ON  
:TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
SBYTE? ->  
:TRIGGER:ENHANCED:I2CBUS:NAIGNORE:  
SBYTE 1

### **:TRIGger:ENHanced:I2CBus:SBHSmode?**

**Function** Queries all settings related to the start byte and high speed mode of the I<sup>2</sup>C bus signal trigger.

**Syntax** :TRIGger:ENHanced:I2CBus:SBHSmode?

**Example** :TRIGGER:ENHANCED:I2CBUS:SBHSMODE? ->  
:TRIGGER:ENHANCED:I2CBUS:SBHSMODE:  
TYPE HSMODE

### **:TRIGger:ENHanced:I2CBus:SBHSmode: TYPE**

**Function** Sets the type of the start byte or high speed mode of the I<sup>2</sup>C bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:I2CBus:SBHSmode:  
TYPE {HSMODE|SBYTE}  
:TRIGger:ENHanced:I2CBus:SBHSmode:TYPE?

**Example** :TRIGGER:ENHANCED:I2CBUS:SBHSMODE:  
TYPE HSMODE  
:TRIGGER:ENHANCED:I2CBUS:SBHSMODE:  
TYPE? ->  
:TRIGGER:ENHANCED:I2CBUS:SBHSMODE:  
TYPE HSMODE

### **:TRIGger:ENHanced:SPIBus?**

**Function** Queries all settings related to the SPI bus signal trigger.

**Syntax** :TRIGger:ENHanced:SPIBus?

**Example** :TRIGGER:ENHANCED:SPIBUS? ->  
:TRIGGER:ENHANCED:SPIBUS:  
BITORDER LSBFIRST;CLOCK:POLARITY FALL;  
SOURCE 1;:TRIGGER:ENHANCED:SPIBUS:CS:  
ACTIVE HIGH;SOURCE 1;:TRIGGER:ENHANCED:  
SPIBUS:DATA1:BYTE 1;CONDITION TRUE;  
DPOSITION 1;PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "00010010";SOURCE 3;:TRIGGER:  
ENHANCED:SPIBUS:DATA2:BYTE 4;  
CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "00010010";SOURCE 3;:TRIGGER:  
ENHANCED:SPIBUS:MODE WIRE3

### **:TRIGger:ENHanced:SPIBus:BITOrder**

**Function** Sets the bit order of the SPI bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:SPIBus:  
BITOrder {LSBFirst|MSBFirst}  
:TRIGger:ENHanced:SPIBus:BITOrder?

**Example** :TRIGGER:ENHANCED:SPIBUS:  
BITORDER LSBFIRST  
:TRIGGER:ENHANCED:SPIBUS:BITORDER? ->  
:TRIGGER:ENHANCED:SPIBUS:  
BITORDER LSBFIRST

### **:TRIGger:ENHanced:SPIBus:CLOCK?**

**Function** Queries all settings related to the clock channel of the SPI bus signal trigger.

**Syntax** :TRIGger:ENHanced:SPIBus:CLOCK?

**Example** :TRIGGER:ENHANCED:SPIBUS:CLOCK? ->  
:TRIGGER:ENHANCED:SPIBUS:CLOCK:  
POLARITY FALL;SOURCE 1

### **:TRIGger:ENHanced:SPIBus:CLOCK: POLarity**

**Function** Sets the polarity of the clock channel of the SPI bus signal trigger or queries the current setting.

**Syntax** :TRIGger:ENHanced:SPIBus:CLOCK:  
POLarity {FALL|RISE}  
:TRIGger:ENHanced:SPIBus:CLOCK:  
POLarity?

**Example** :TRIGGER:ENHANCED:SPIBUS:CLOCK:  
POLARITY FALL  
:TRIGGER:ENHANCED:SPIBUS:CLOCK:  
POLARITY? ->  
:TRIGGER:ENHANCED:SPIBUS:CLOCK:  
POLARITY FALL

**:TRIGger:ENHanced:SPIBus:CLOCK:SOURce**

Function Sets the clock channel of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:SPIBus:CLOCK:  
SOURce {<NRf>}  
:TRIGger:ENHanced:SPIBus:CLOCK:SOURce?  
<NRf> = 1 to 4

Example :TRIGGER:ENHANCED:SPIBUS:CLOCK:SOURCE 1  
:TRIGGER:ENHANCED:SPIBUS:CLOCK:  
SOURCE? ->  
:TRIGGER:ENHANCED:SPIBUS:CLOCK:SOURCE 1

**:TRIGger:ENHanced:SPIBus:CS?**

Function Queries all settings related to the chip select channel of the SPI bus signal trigger.

Syntax :TRIGger:ENHanced:SPIBus:CS?

Example :TRIGGER:ENHANCED:SPIBUS:CS? ->  
:TRIGGER:ENHANCED:SPIBUS:CS:ACTIVE  
HIGH;SOURCE 1

**:TRIGger:ENHanced:SPIBus:CS:ACTive**

Function Sets the active level of the chip select channel of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:SPIBus:CS:  
ACTive {HIGH|LOW}  
:TRIGger:ENHanced:SPIBus:CS:ACTive?

Example :TRIGGER:ENHANCED:SPIBUS:CS:ACTIVE HIGH  
:TRIGGER:ENHANCED:SPIBUS:CS:ACTIVE? ->  
:TRIGGER:ENHANCED:SPIBUS:CS:ACTIVE HIGH

**:TRIGger:ENHanced:SPIBus:CS:SOURce**

Function Sets the chip select channel of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:SPIBus:CS:  
SOURce {<NRf>}  
:TRIGger:ENHanced:SPIBus:CS:SOURce?  
<NRf> = 1 to 4

Example :TRIGGER:ENHANCED:SPIBUS:CS:SOURCE 1  
:TRIGGER:ENHANCED:SPIBUS:CS:SOURCE? ->  
:TRIGGER:ENHANCED:SPIBUS:CS:SOURCE 1

**:TRIGger:ENHanced:SPIBus:DATA<x>?**

Function Queries all settings related to the data of the SPI bus signal trigger.

Syntax :TRIGger:ENHanced:SPIBus:DATA<x>?  
<x> = 1 or 2

Example :TRIGGER:ENHANCED:SPIBUS:DATA1? ->  
:TRIGGER:ENHANCED:SPIBUS:DATA1:BYTE 1;  
CONDITION TRUE;DPOSITION 1;  
PATTERN1 "00010010";  
PATTERN2 "00110100";  
PATTERN3 "01010110";  
PATTERN4 "00010010";SOURCE 3

Description DATA2 is valid when :TRIGger:ENHanced:  
SPIBus:MODE WIRE4 is specified.

**:TRIGger:ENHanced:SPIBus:DATA<x>:****BYTE**

Function Sets the number of bytes of the data of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:SPIBus:DATA<x>:  
BYTE {<NRf>}  
:TRIGger:ENHanced:SPIBus:DATA<x>:BYTE?  
<x> = 1 or 2  
<NRf> = 1 to 4

Example :TRIGGER:ENHANCED:SPIBUS:DATA1:BYTE 1  
:TRIGGER:ENHANCED:SPIBUS:DATA1:BYTE? ->  
:TRIGGER:ENHANCED:SPIBUS:DATA1:BYTE 1

**:TRIGger:ENHanced:SPIBus:DATA<x>:****CONDition**

Function Sets the determination method (match or not match) of the data of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:SPIBus:DATA<x>:  
CONDition {FALSE|TRUE}  
:TRIGger:ENHanced:SPIBus:DATA<x>:  
CONDition?  
<x> = 1 or 2

Example :TRIGGER:ENHANCED:SPIBUS:DATA1:  
CONDITION TRUE  
:TRIGGER:ENHANCED:SPIBUS:DATA1:  
CONDITION? ->  
:TRIGGER:ENHANCED:SPIBUS:DATA1:  
CONDITION TRUE

**:TRIGger:ENHanced:SPIBus:DATA<x>:****DPOSITion**

Function Sets the pattern comparison start position of the data of the SPI bus signal trigger or queries the current setting.

Syntax :TRIGger:ENHanced:SPIBus:DATA<x>:  
DPOSITion {<NRf>}  
:TRIGger:ENHanced:SPIBus:DATA<x>:  
DPOSITion?  
<x> = 1 or 2  
<NRf> = 0 to 9999

Example :TRIGGER:ENHANCED:SPIBUS:DATA1:  
DPOSITION 1  
:TRIGGER:ENHANCED:SPIBUS:DATA1:  
DPOSITION? ->  
:TRIGGER:ENHANCED:SPIBUS:DATA1:  
DPOSITION 1

## 4.5 TRIGGER Group

### **:TRIGGER:ENHANCED:SPIBUS:DATA<x>:**

#### **HEXA<x>**

**Function** Sets the data of the SPI bus signal trigger in hexadecimal notation.

**Syntax** :TRIGGER:ENHANCED:SPIBUS:DATA<x>:  
HEXA<x> {<String>}  
<x> of DATA<x> = 1 or 2  
<x> of HEXA<x> = 1 to 4  
<String> = 2 characters by combining '0' to 'F' and 'X'

**Example** :TRIGGER:ENHANCED:SPIBUS:DATA1:  
HEXA1 "AB"

### **:TRIGGER:ENHANCED:SPIBUS:DATA<x>:**

#### **PATTERN<x>**

**Function** Sets the data of the SPI bus signal trigger in binary notation or queries the current setting.

**Syntax** :TRIGGER:ENHANCED:SPIBUS:DATA<x>:  
PATTERN<x> {<String>}  
:TRIGGER:ENHANCED:SPIBUS:DATA<x>:  
PATTERN<x>?  
<x> of DATA<x> = 1 or 2  
<x> of <PATTERN x> = 1 to 4  
<String> = 8 characters by combining '0', '1', and 'X'

**Example** :TRIGGER:ENHANCED:SPIBUS:DATA1:  
PATTERN1 "10101011"  
:TRIGGER:ENHANCED:SPIBUS:DATA1:  
PATTERN1? ->  
:TRIGGER:ENHANCED:SPIBUS:DATA1:  
PATTERN1 "10101011"

### **:TRIGGER:ENHANCED:SPIBUS:DATA<x>:**

#### **SOURCE**

**Function** Sets the source channel of the data of the SPI bus signal trigger or queries the current setting.

**Syntax** :TRIGGER:ENHANCED:SPIBUS:DATA<x>:  
SOURCE {<NRf>}  
:TRIGGER:ENHANCED:SPIBUS:DATA<x>:  
SOURCE?  
<x> = 1 or 2  
<NRf> = 1 to 4

**Example** :TRIGGER:ENHANCED:SPIBUS:DATA1:SOURCE 1  
:TRIGGER:ENHANCED:SPIBUS:DATA1:  
SOURCE? ->  
:TRIGGER:ENHANCED:SPIBUS:DATA1:SOURCE 1

### **:TRIGGER:ENHANCED:SPIBUS::MODE**

**Function** Sets the wiring system of the SPI bus signal trigger (three-wire or four-wire) or queries the current setting.

**Syntax** :TRIGGER:ENHANCED:SPIBUS:  
MODE {WIRE3|WIRE4}  
:TRIGGER:ENHANCED:SPIBUS:MODE?

**Example** :TRIGGER:ENHANCED:SPIBUS:MODE WIRE3  
:TRIGGER:ENHANCED:SPIBUS:MODE? ->  
:TRIGGER:ENHANCED:SPIBUS:MODE WIRE3

### **:TRIGGER:SOURCE:CHANNEL<x>:LEVEL**

**Function** Sets the trigger level of the channel or queries the current setting.

**Syntax** :TRIGGER:SOURCE:CHANNEL<x>:  
LEVEL {<Voltage>|<Current>}  
:TRIGGER:SOURCE:CHANNEL<x>:LEVEL?  
<x> = 1 to 4  
<Voltage> and <Current> = See the *User's Manual (IM701310-01E)*.

**Example** :TRIGGER:SOURCE:CHANNEL1:LEVEL 1V  
:TRIGGER:SOURCE:CHANNEL1:LEVEL? ->  
:TRIGGER:SOURCE:CHANNEL1:  
LEVEL 1.000E+00

**Description** This command applies to the channel corresponding to the source specified by the following commands.

- :TRIGGER:ENHANCED:I2CBUS:CLOCK:SOURCE
- :TRIGGER:ENHANCED:I2CBUS:DATA:SOURCE
- :TRIGGER:ENHANCED:SPIBUS:CLOCK:SOURCE
- :TRIGGER:ENHANCED:SPIBUS:CS:SOURCE
- :TRIGGER:ENHANCED:SPIBUS:DATA[1-2]:SOURCE

### **:TRIGGER:SOURCE:CHANNEL<x>:STATE**

**Function** Sets the condition to be satisfied of the channel or queries the current setting.

**Syntax** :TRIGGER:SOURCE:CHANNEL<x>:  
STATE {DONTcare|HIGH|LOW}  
:TRIGGER:SOURCE:CHANNEL<x>:STATE?  
<x> = 1 to 4

**Example** :TRIGGER:SOURCE:CHANNEL1:STATE HIGH  
:TRIGGER:SOURCE:CHANNEL1:STATE? ->  
:TRIGGER:SOURCE:CHANNEL1:STATE HIGH

**Description** • This command is valid when :TRIGGER:TYPE I2CBUS.

### **:TRIGGER:TYPE**

**Function** Sets the trigger type or queries the current setting.

**Syntax** :TRIGGER:TYPE {CANBUS|EDGE|EICYCLE|  
EIDelay|EISequence|EOR|EQualify|I2CBUS|  
PQualify|PSTATE|PULSE|SPATtern|SPIBUS|  
STATE|TV}  
:TRIGGER:TYPE?

**Example** :TRIGGER:TYPE CANBUS  
:TRIGGER:TYPE? ->  
:TRIGGER:TYPE CANBUS

## 5.1 I<sup>2</sup>C Bus Signal Analysis Function

### Applicable Bus

Item	Specifications
I <sup>2</sup> C bus	Bus transfer rate: Up to 3.4 Mbits/s Address mode: 7 bits/10 bits

### Trigger Function

Item	Specifications
Trigger source	CH1 to CH4
I <sup>2</sup> C bus signal trigger	<p>Select from the following five trigger types.</p> <ul style="list-style-type: none"> <li>•Every Start: Activate a trigger when a start condition is detected</li> <li>•Address&amp;Data: Activate a trigger based on the comparison against the specified address and data</li> <li>•Non-ACK: Activate a trigger when Nack is detected</li> <li>•General Call: Activate a trigger based on the comparison against the second byte pattern of the general call address</li> <li>•Start Byte/HS Mode: Activate a trigger on the start byte or the master address of HS mode</li> </ul> <p>The address type of the Address&amp;Data trigger can be selected from the following three types.</p> <ul style="list-style-type: none"> <li>•7bit address</li> <li>•7bit + Sub Adr</li> <li>•10bit Address</li> </ul>

### Analysis Function

Item	Specifications
Signal input	Select from CH1 to CH4 or M1 to M4.
Number of data bytes that can be analyzed	40000 bytes max.
Display of the analysis results	Displays No. (analysis number and start/stop conditions), Time (time from the analysis reference), Binary (binary display of the analysis data), Hex (hexadecimal display of analysis data), and Ack (Acknowledge bit condition).
Zoom link	Moves the zoom position (the center of the zoom box) to the head of the byte highlighted in the analysis result list. Changing the zoom position causes the highlighting in the analysis result list to also move.
Saving of the data of the analysis results list	Saves the list of detailed analysis results to a file in CSV format (.csv extension).

### Search Function

Item	Specifications
Data search	Set the address pattern, data pattern, and Acknowledge bit condition and search the waveform. If a waveform that matches the condition is found, the zoom box moves to that point and displays the specified waveform.

## 5.2 CAN Bus Signal Analysis Function

### Applicable CAN Bus

Item	Specifications
CAN bus	CAN Version 2.0B
Baud rate	Set any of the following bit rates: 1 M, 500 k, 250 k, 125 k, 83.3 k[bps], or an arbitrary bit rate from 10 k to 1 M[bps] (0.1 kbps resolution). Supports High speed CAN (ISO11898) and Low speed CAN (ISO11519-2).

### Trigger Function

Item	Specifications
Trigger source	Select CH1 to CH4.
CAN bus signal trigger	Select from the following five trigger modes. <ul style="list-style-type: none"><li>• SOF: Activates a trigger on the SOF (Start of Frame).</li><li>• Error Frame: Activates a trigger on an error frame.</li><li>• ID Std/Data: Activates a trigger on a data frame or remote frame (ID: standard format).</li><li>• ID Ext/Data: Activates a trigger on a data frame or remote frame (ID: extended format).</li><li>• ID/Data OR: Activates a trigger on the OR conditions of four types of data frames or remote frames. Select standard or extended format for each ID.</li></ul>

### Analysis Function

Item	Specifications
Signal input	Select a channel from CH1 to CH4 and M1 to M4.
Number of frames that can be analyzed	Up to 3000 frames
Analyzed frames	Data frame, remote frame, error frame, and overload frame.
Display of the analysis results	<ul style="list-style-type: none"><li>• Simple display Displays the analysis number (No.), frame type (Frame), ID in hexadecimal notation, Data in hexadecimal notation, and ACK slot state.</li><li>• Detail display Displays the analysis number (No.), frame type (Frame), time from the trigger position (Time (ms)), ID in hexadecimal notation, DLC in hexadecimal notation, Data in binary notation (Data (Bin)), Data in hexadecimal notation (Data), CRC sequence in hexadecimal notation, and ACK slot state.</li></ul>
Zoom link	<ul style="list-style-type: none"><li>• Zoom link Moves the zoom position (the center of the zoom box) to the head of the frame highlighted in the analysis result list. Changing the zoom position causes the highlighting in the analysis result list to also move.</li><li>• Field jump When the zoom link function is enabled, the zoom position can be moved to the head of the specified field of the frame that is highlighted in the analysis result list. Select the field from SOF, ID, Control Field, Data Field, CRC, or ACK.</li></ul>
Saving of the data of the analysis results list	Saves the data of the simple display and detail display of the analysis result list in CSV format (.csv extension).

### Search Function

Item	Specifications
Data search	Search the waveform by specifying a field or frame condition. If a waveform that matches the condition is found, the zoom box moves to that point and displays the specified waveform in the zoom window.

### Stuff Bit Computation Function

Item	Specifications
Stuff bit computation	Extracts stuff bits from the CAN bus waveform and displays them as a MATH waveform (MATH1 to MATH4).

## 5.3 SPI Bus Signal Analysis Function

### Trigger Function

Item	Specifications
Trigger source	CH1 to CH4
SPI bus signal trigger	Activate a trigger by comparing data from an arbitrary byte counts after the assertion of the CS. The length of data that is compared can be set to 1 to 4 bytes.

### Analysis Function

Item	Specifications
Number of data bytes that can be analyzed	40000 bytes max.
Display of the analysis results	Detailed analysis result list display. Displays No. (analysis number), Time (time from the analysis reference point), Dt1 (hexadecimal or binary display of the Data 1 value), Dt2 (hexadecimal or binary display of the Data 2 value), CS (CS signal status or the CS signal name with high precedence).
Zoom Link	Moves the zoom position (the center of the zoom box) to the head of the byte highlighted in the analysis result list. Changing the zoom position causes the highlighting in the analysis result list to also move.
Saving of the data of the analysis results list	Saves the list of detailed analysis results to a file in CSV format (.csv extension).

### Search Function

Item	Specifications
Data search	Search the waveform by specifying a data pattern. If a waveform that matches the pattern is found, the zoom box moves to that point and displays the specified waveform.

# Index

## A Page

ACK Slot .....	2-13
Active .....	3-13, 3-14
Address & Data Trigger .....	1-8
Address Type .....	1-8
ADR & DATA .....	1-8, 1-23
Analysis Condition	
CAN .....	2-21
I <sup>2</sup> C .....	1-17
SPI .....	3-13
Analysis Data List	
CAN .....	2-22
I <sup>2</sup> C .....	1-18
SPI .....	3-15
Analysis Function	
CAN .....	2-1
I <sup>2</sup> C .....	1-1
SPI .....	3-2
ANALYSIS Group .....	4-1, 4-15
Analysis Number .....	3-15, 3-16
CAN .....	2-22, 2-23
I <sup>2</sup> C .....	1-18, 1-19
Analysis Range	
CAN .....	2-22
I <sup>2</sup> C .....	1-18
SPI .....	3-15
Analysis Reference Point	
CAN .....	2-21
I <sup>2</sup> C .....	1-18
SPI .....	3-15
Analysis Result List	
CAN .....	2-22
I <sup>2</sup> C .....	1-18
SPI .....	3-15
Analyzed Data	
CAN .....	2-22
I <sup>2</sup> C .....	1-18
SPI .....	3-14

## B Page

Big Endian .....	2-12
Bit Order .....	3-7, 3-13
Bitrate .....	2-10, 2-21, 2-31
Bus Level .....	2-14, 2-21, 2-31
Byte Order .....	2-12

## C Page

CAN Bus Signal Analysis Function .....	2-1, 5-2
Chip Select Signal .....	3-13
Clock Channel .....	1-17
Clock Signal .....	3-7, 3-14
Comparison Data .....	2-12
Connecting the Probe .....	2-2
Coupling	
CAN .....	2-14
I <sup>2</sup> C .....	1-13
SPI .....	3-7
CS .....	3-7, 3-13

## D Page

Data Channel .....	1-17
Data Format	
CAN .....	2-32
I <sup>2</sup> C .....	1-29
SPI .....	3-22
Data Frame .....	2-11, 2-15, 2-22
Detail Display	
CAN .....	2-23
I <sup>2</sup> C .....	1-19
SPI .....	3-16
Differential Probe .....	2-2
DLC .....	2-11

## E Page

Error Frame .....	2-10, 2-16, 2-22, 2-28
Error Message	
CAN .....	2-33
I <sup>2</sup> C .....	1-30
SPI .....	3-23
Every Start .....	1-8, 1-23

## F Page

Field Jump .....	2-24
------------------	------

## G Page

General Call .....	1-23
General Call Trigger .....	1-10

## H Page

High Speed CAN .....	2-2
HS Mode .....	1-12
Hysteresis	
CAN .....	2-21, 2-31
I <sup>2</sup> C .....	1-17
SPI .....	3-13, 3-14

## I Page

I <sup>2</sup> C Bus Signal Analysis Function .....	1-1, 5-1
ID Ext/Data .....	2-10, 2-11, 2-28
ID Std/Data .....	2-10, 2-11, 2-28
ID/Data OR .....	2-10, 2-14

## L Page

Level	
CAN .....	2-14, 2-21, 2-31
I <sup>2</sup> C .....	1-17
SPI .....	3-13, 3-14
Little Endian .....	2-12
Logic .....	1-13
Low Speed CAN .....	2-2
LSB .....	2-13



## Index

### **M** **Page**

MATH Group .....	4-2, 4-22
Message	
CAN .....	2-33
I <sup>2</sup> C .....	1-30
SPI .....	3-23
MSB .....	2-13

### **N** **Page**

Nack Trigger .....	1-10
NON ACK .....	1-10, 1-23

### **O** **Page**

Overload Frame .....	2-22
----------------------	------

### **R** **Page**

Recessive .....	2-14, 2-21, 2-31
Ref Point	
CAN .....	2-21
I <sup>2</sup> C .....	1-18
SPI .....	3-15
Remote Frame .....	2-11, 2-16, 2-22
RTR .....	2-11

### **S** **Page**

Sample Point .....	2-10, 2-21, 2-31
Saved Data	
CAN .....	2-32
I <sup>2</sup> C .....	1-29
SPI .....	3-22
Saving the Data of the Analysis Result List	
CAN .....	2-32
I <sup>2</sup> C .....	1-25
SPI .....	3-22
SCL .....	1-17
SDA .....	1-17
Search Condition	
CAN .....	2-28
I <sup>2</sup> C .....	1-23
SPI .....	3-20
Search Function	
CAN .....	2-1
I <sup>2</sup> C .....	1-1
SPI .....	3-2
SEARCh Group .....	4-3, 4-23
Search Mode	
CAN .....	2-28
I <sup>2</sup> C .....	1-23
Search Point	
CAN .....	2-28
I <sup>2</sup> C .....	1-23
SPI .....	3-21
Search Start Point	
CAN .....	2-28
I <sup>2</sup> C .....	1-23
SPI .....	3-20
Simple Display	
CAN .....	2-22
I <sup>2</sup> C .....	1-18
SPI .....	3-15

Skip Mode	
CAN .....	2-28
I <sup>2</sup> C .....	1-23
SPI .....	3-20
SOE .....	2-10, 2-28
Source Channel	
CAN .....	2-14, 2-21
I <sup>2</sup> C .....	1-12
SPI .....	3-7
SPI Bus Signal Analysis Function .....	3-1, 5-3
SS .....	3-13
Start Byte .....	1-12
Start Byte/HS Mode .....	1-23
Start Byte/HS Mode Trigger .....	1-12
Storage Condition	
CAN .....	2-32
I <sup>2</sup> C .....	1-27
SPI .....	3-22
Stuff Bit .....	2-30
Stuff Bit Computation .....	2-1, 2-29

### **T** **Page**

Three-Wire or Four-Wire .....	3-7, 3-13
Trigger Condition	
CAN .....	2-10
SPI .....	3-7
Trigger Coupling	
CAN .....	2-14
I <sup>2</sup> C .....	1-13
SPI .....	3-7
Trigger Function	
CAN .....	2-1
I <sup>2</sup> C .....	1-1
SPI .....	3-1
TRIGger Group .....	4-6, 4-35
Trigger Level	
CAN .....	2-14
I <sup>2</sup> C .....	1-13
SPI .....	3-7
Trigger Mode	
CAN .....	2-10
I <sup>2</sup> C .....	1-7
Trigger Point	
CAN .....	2-15
SPI .....	3-8

### **V** **Page**

Viewing Search Point	
CAN .....	2-28
I <sup>2</sup> C .....	1-23
SPI .....	3-21

### **Z** **Page**

Zoom Link	
CAN .....	2-24
I <sup>2</sup> C .....	1-19
SPI .....	3-16