

---

**Operation  
Guide**



**MW100  
Data Acquisition Unit**

---

---

# Contents

<b>Checking the Contents of the Package</b> .....	<b>5</b>
<b>Introduction to Functions</b> .....	<b>10</b>
Overview of the MW100 Data Acquisition Unit .....	10
Overview of MW100 Viewer Software .....	11
Address Setting Software .....	11
Viewer.....	12
Calibrator .....	12
Flow of Operations during Installation .....	13
<b>Connecting to a Network</b> .....	<b>14</b>
Connecting an Ethernet Cable to the Main Module .....	14
Checking the Communication Status.....	14
Connection to the PC.....	14
<b>Connecting the Main Module to a PC</b> .....	<b>15</b>
Ethernet Connection .....	15
<b>Entering Settings on the MW100 Using a Browser</b> .....	<b>17</b>
MW100 System Settings .....	17
Measurement Groups and Measurement Module Settings .....	18
Settings for Recording to CF Card.....	19
Recording Channel Settings .....	19
Measuring Interval and Range Settings (for the Universal Input Module) .....	20
Alarm and Relay Settings .....	21
<b>Changing Monitor Screen Display Conditions</b> .....	<b>22</b>
Tag Settings .....	22
Setting Messages .....	22
Display Scale Settings .....	23
Display Color Settings .....	24
Display Group Settings .....	24
<b>Starting and Stopping Measurement and Recording</b> .....	<b>25</b>
Starting Measurement .....	25
Starting Recording .....	26
Stopping Recording .....	26
Stopping Measurement.....	26
<b>Viewing Measured Data on the Monitor Screen and Starting/Stopping Recording</b> .....	<b>27</b>
Transferring Measured Data to the FTP Server.....	30
<b>Viewing Measured Data on the Viewer Software</b> .....	<b>31</b>
Displaying Data.....	31
Changing the Display on the Waveform Display Window.....	32
Changing the Display Using the Toolbar.....	32
Changing the Display Using the Menu .....	32
Changing the Display Using the Display Setup Window .....	33
Numerical Display.....	33
Reading Values Using the Cursor.....	34
Statistical Computation over an Area of Measured/Computed Data .....	34
Alarm/Mark List.....	35
Setting the Contents to Be Printed .....	36
Converting Data Formats.....	36

# User Registration

Thank you for purchasing YOKOGAWA products.

We invite you to register your products in order to receive the most up to date product information. To register, visit the following URL, or click the “Product Registration” button in the opening screen of the Manual CD-ROM.

***<http://www.yokogawa.com/ns/reg/>***

---

## Foreword

Thank you for purchasing the MW100 Data Acquisition Unit.

This manual provides an overview of the operating procedures of the MW100 Data Acquisition Unit, and the basic operating procedures of the Viewer software. To ensure correct use, please read this manual thoroughly before beginning operation.

The following six manuals relating to the MW100 Data Acquisition Unit are provided in addition to this one. Read them along with this manual. The MW100 User's Manual (IM MW100-01E), MW100 Viewer Software User's Manual (IM MW180-01E), MW100 Communication Command Manual (IM MW100-17E), and this manual (IM MW100-02E) are all available on the MW100 Manual CD-ROM.

Manual Title	Manual No.	Description
MW100 Data Acquisition Unit User's Manual	IM MW100-01E	Explains the MW100 Data Acquisition Unit functions, installation and wiring procedures, precautions, and browser operations.
MW100 Communication Command Manual	IM MW100-17E	Lists and explains usage of the commands that can be used with the MW100 Main Module.
Precautions on the Use of the MX100/MW100	IM MX100-71E	Explains precautions during use of the MX100/MW100 Data Acquisition Unit
MX100 Data Acquisition Unit Installation and Connection Guide	IM MX100-72E	Gives an overview of installation and wiring procedures for the MW100 Data Acquisition Unit
Control of pollution caused by MX100/MW100 products	IM MX100-91C	Describes control of pollution caused by the product.
MW100 Viewer Software User's Manual	IM MW180-01E	Explains the functions and operations of the Viewer software that comes standard with the MW100 Main Module.

## Notes

- This manual describes style number S3 of the MW100 Data Acquisition Unit. It also describes release number R3.01 of the MW100 Viewer Software.
- Every effort has been made in the preparation of this manual to ensure the accuracy of its contents. However, should you have any questions or find any errors, please contact your nearest YOKOGAWA representative, dealer, or sales office.
- This user's manual does not cover the handling and operating procedures of Windows.
- Copying or reproducing all or any part of the contents of this manual without YOKOGAWA's permission is strictly prohibited.
- The TCP/IP software and related documentation for this product was developed and created by Yokogawa based on BSD Networking Software Release 1, licensed from the University of California.

## Trademarks

- DAQMASTER is a registered trademarks of Yokogawa Electric Corporation.
- Microsoft and Windows are registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.
- Adobe and Acrobat are registered trademarks or trademarks of Adobe Systems Incorporated.
- Company and product names that appear in this manual are registered trademarks or trademarks of their respective holders.
- The company and product names used in this manual are not accompanied by the registered trademark or trademark symbols (® and ™).

## Revisions

1st Edition: June, 2005

2nd Edition: October, 2006


3rd Edition: October, 2007

# Checking the Contents of the Package

Unpack the box and check the contents before operating the instrument. If some of the contents are not correct, or if any items are missing or damaged, contact the dealer from whom you purchased them.

## Checking the Model and Suffix Code

Check the model and suffix code on the name plate indicated in the figure below.

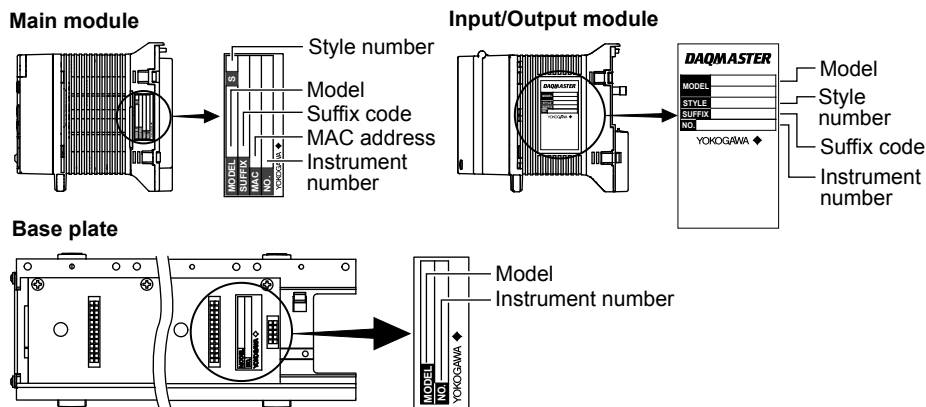

### Note

When contacting the dealer from which you purchased the instrument, please give them the NO. (instrument number) on the name plate.

## Main Module

Model	Suffix Code	Description
MW100		Main module
Language	-E	English (comes with an English manual) <sup>*1</sup>
Supply voltage	-1	100 VAC-240 VAC
	-2	12 VDC-28VDC, with AC adapter <sup>*2</sup>
	-3	12 VDC-28VDC, without AC adapter <sup>*3</sup>
Power supply and power cord	-D	AC power: 3-pin inlet, UL/CSA Standard power cord DC power: Screw terminal, UL/CSA cable for AC adapter
	-F	AC power: 3-pin inlet, VDE Standard power cord DC power: Screw terminal, VDE cable for AC adapter
	-R	AC power: 3-pin inlet, AS Standard power cord DC power: Screw terminal, AS cable for AC adapter
	-Q	AC power: 3-pin inlet, BS Standard power cord DC power: Screw terminal, BS cable for AC adapter
	-H	AC power: 3-pin inlet, GB (CCC) Standard power cord DC power: Screw terminal, GB (CCC) cable for AC adapter
	-W	Screw terminal, power supply cord not included <sup>*2, *3</sup>
Options	/C2	RS-232 communications interface <sup>*4, *5</sup>
	/C3	RS-422A/485 communications interface <sup>*4, *5</sup>
	/M1	Mathematical function <sup>*5, *6</sup>
	/M3	Report function
	/SL1	10ch Quick Start Package <sup>*7</sup>
	/SL2	20ch Quick Start Package <sup>*7</sup>
	/SL3	30ch Quick Start Package <sup>*7</sup>

\*1 Displays Celsius or Fahrenheit, Daylight savig time can be set.

\*2 "W" cannot be selected with "-2."

\*3 "-3" can only be selected with "W"

\*4 "/C2" and "/C3" may not be selected together.

\*5 "/C2" or "/C3" must be selected to use the Modbus/RTU slave function. Also, "/M1" must be selected for use of the Modbus/RTU master function.

\*6 "/M1" must be selected to use the Modbus/TCP client function.

\*7 "/SL1", "/SL2", and "/SL3" may not be selected together.

## Universal Input Module, DCV/TC/DI Input Module, and Four-Wire RTD Resistance Input Module

Model	Suffix Code	Description
MX110		
Input type	-UNV	For DCV/TC/DI/3-wire RTD input
	-VTD	For DCV/TC/DI input
	-V4R	For DCV/DI/4-wire RTD/4-wire resistance input
Number of channels and measurement interval	-H04 <sup>*1</sup>	4-CH, high-speed measurement (minimum measurement interval: 10 ms)
	-M06 <sup>*1</sup>	6-CH, medium-speed measurement (minimum measurement interval: 100 ms)
	-M10 <sup>*1</sup>	10-CH, medium-speed measurement (minimum measurement interval: 100 ms)
	-L30 <sup>*1</sup>	30-CH, medium-speed measurement (minimum measurement interval: 500 ms)
Options	/NC <sup>*2</sup>	Without the plate with the clamp terminals
	/H3 <sup>*3</sup>	M3 screw terminals

\*1 “-H04” or “-M10” must be selected if “-UNV” is selected. “-M06” must be selected if “-V4R” is selected. “-VTD” must be selected if “-L30” is selected.

\*2 The “/NC” option can be specified only when “-M10” is specified.

\*3 The “/H3” option can be specified only when “-L30” is specified.

## Strain Input Module

Model	Suffix Code	Description
MX112		
Input type	-B12	Internal bridge resistance: 120 Ω
	-B35	Internal bridge resistance: 350 Ω
	-NDI	NDIS connector for connections to an external bridge head
Number of channels and measurement interval	-M04	4-CH, medium-speed measurement (minimum measurement and measurement interval: 100 ms)

## Pulse Input Module

Model	Suffix Code	Description
MX114		
Input type	-PLS	Non-voltage contact, 5-V logic, open collector input
Number of channels and measurement interval	-M10	10-CH, medium-speed measurement (minimum measurement interval: 100 ms)
Options	/NC	Without the plate with the clamp terminals

## Digital Input Module

Model	Suffix Code	Description
MX115		
Input type	-D05	Non-voltage contact, 5-V logic, open collector input
	-D24	24 V logic
Number of channels and measurement interval	-H10	10-CH, high-speed measurement (minimum measurement and measurement interval: 10 ms)
Options	/NC	Without the plate with the clamp terminals

## Analog Output Module

Model	Suffix Code	Description
MX120		
Output type	-VAO	Voltage/current output
	-PWM	Pulse width modulation output
Number of channels and output update interval	-M08	8-CH, minimum output update interval: 100 ms

## Digital Output Module

Model	Suffix Code	Description
MX125		
Output type	-MKC	A contact output
Number of channels and output update interval	-M10	10-CH, minimum output update interval: 100 ms

## Base Plate


Model	Suffix Code	Description
MX150		Includes two brackets for DIN rail mount
Base type	-1 to -6*	The value of the suffix code corresponds to the maximum number of input output modules that can be installed. MX150-6 is for one main module, and six input/output modules.

\* One unit of the MX110-VTD-L30 requires three slots worth of space when installing.

## Standard Accessories


The following standard accessories are supplied with the main module. Check that all contents are present and that they are undamaged.

**Power Cord (one of the following power cords is supplied according to the instrument's suffix codes)**

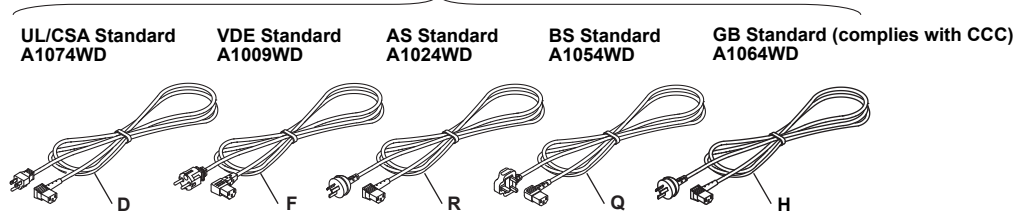


Note: Not included when screw terminals are specified for the power section (Suffix code: W).

AC adapter and Power cord\*1  
Model: 772075



**\*1 Power Cord for AC adapter (one of the following power cords is supplied according to the instrument's suffix codes)**

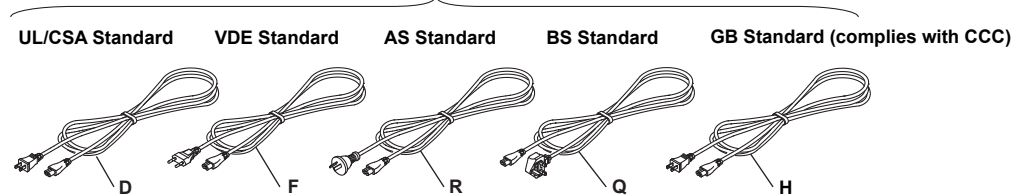

Note: Not included when screw terminals are specified for the power section (Suffix code: W).

MW100 Viewer Software  
Model: MW180-1




MW100 Manual CD-ROM\*2  
Part number: B8724XA



\*2 Includes:


- MW100 Data Acquisition Unit User's Manual (IM MW100-01E)
- This manual (IM MW100-02E)
- MW100 Communication Command Manual (IM MW100-17E)
- MW100 Viewer Software User's Manual (IM MW180-01E)

Paper Manuals



- MW100 Data Acquisition Unit Operation Guide (IM MW100-02E)
- Precautions on the Use of the MX100/MW100 Data Acquisition Unit (IM MX100-71E)
- MX100/MW100 Data Acquisition Unit Installation and Connection Guide (IM MX100-72E)
- Control of pollution caused by MX100/MW100 products (IM MX100-91C)

Bracket for base plate  
Part number: B8724EF



Screw for bracket  
Part number: B9988DL



## Optional Accessories (Sold Separately)

### AC adapter

No.	Name	Model	Basic Suffix Code	Min. Q'ty	Note
1	AC adapter	772075			
	Power supply code		-D	1	Cable for UL/CSA
			-F	1	Cable for VDE
			-R	1	Cable for AS
			-Q	1	Cable for BS
			-H	1	Cable for GB (CCC)


### Terminals

No.	Name	Model	Min. Q'ty	Note
2	10-CH screw terminal block (with RJC)	772061	1	Dedicated to the MX110-UNV-M10/ MX114-PLS-M10/MX115-D05-H10/ MX115-D24-H10
3	Connection cable between the input module and screw terminal block	772062-050	1	Cable length: 50 cm <sup>*1</sup>
4	Connection cable between the input module and screw terminal block	772062-100	1	Cable length: 100cm <sup>*1</sup>
5	Plate with clamp terminals (with RJC)	772063	1	Dedicated to the MX110-UNV-M10/ MX114-PLS-M10/MX115-D05-H10/ MX115-D24-H10
6	Clamp terminal	772064	1	Dedicated to the MX110-UNV-H04
7	Clamp terminal	772065	1	Dedicated to the MX120-VAO-M08/ MX120-PWM-M08/MX125-MKC-M10
8	Connector cover	772066	1	For empty slots with no module installed
9	Plate with clamp terminals	772067	1	Dedicated to the MX110-V4R-M06
10	Plate with clamp terminals (Built in bridge: 120 Ω)	772068	1	Dedicated to the MX112-B12-M04 <sup>*2</sup>
11	Plate with clamp terminals (Built in bridge: 350 Ω)	772069	1	Dedicated to the MX112-B35-M04 <sup>*2</sup>
12	Plate with screw terminal	772080	1	Dedicated to the MX110-UNV-M10/ MX114-PLS-M10/MX115-D05-H10/ MX115-D24-H10
13	Plate with screw terminal for current (Built-in shunt resistor of 10 Ω)	772081	1	Dedicated to the MX110-UNV-M10
14	Plate with screw terminal for current (Built-in shunt resistor of 100 Ω)	772082	1	Dedicated to the MX110-UNV-M10
15	Plate with screw terminal for current (Built-in shunt resistor of 250 Ω)	772083	1	Dedicated to the MX110-UNV-M10

\*1 For the 772062, only applies from MX110-UNV-M10 to screw terminal block (772061), MX114-PLS-M10 to screw terminal block (772061), MX115-D05-H10 to screw terminal block (772061), and MX115-D24-H10 to screw terminal block (772061).

\*2 772068 is only applicable to MX112-B35-M04. 772069 is only applicable to MX112-B12-M04.



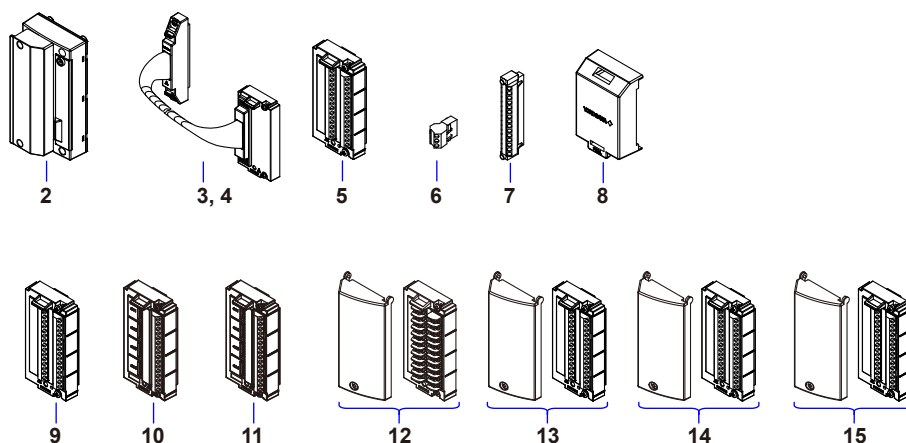

**Shunt resistor**

No.	Name	Model	Min. Q'ty	Note
16	Shunt resistor (for the clamp terminal)	438920	1	Resistance: 250 $\Omega$ ±0.1%
17	Shunt resistor (for the clamp terminal)	438921	1	Resistance: 100 $\Omega$ ±0.1%
18	Shunt resistor	438922	1	Resistance: 10 $\Omega$ ±0.1%
19	Shunt resistor	415920	1	Resistance: 250 $\Omega$ ±0.1%
20	Shunt resistor	415921	1	Resistance: 100 $\Omega$ ±0.1%
21	Shunt resistor	415922	1	Resistance: 10 $\Omega$ ±0.1%

**Memory card**

No.	Name	Model	Min. Q'ty	Note
22	Adapter for CompactFlash card	772090	1	
23	CompactFlash card	772091	1	128 MB*
24	CompactFlash card	772092	1	256 MB*
25	CompactFlash card	772093	1	512 MB*
26	CompactFlash card	772094	1	1 GB*

\* Operating temperature range: -40 to 85°C

**Software Application (Sold Separately)**

No.	Name	Model	Note
1	GateMX/MW	WX1	MX100/MW100 Gate software for connecting to DAQLOGGER data acquisition software.

**Style Upgrade Kit (Sold Separately)**

No.	Name	Model	Note
1	Style upgrade kit for the MW100	772050-02	Upgrades the MW100 from Style 2 to Style 3.

# Introduction to Functions

For details on individual functions, see one of the following user's manuals located on the enclosed CD-ROM: MW100 Data Acquisition Unit User's Manual (IM MW100-01E), MW100 Communication Command Manual (IM MW100-17E), or MW100 Viewer Software User's Manual (IM MW180-01E).

## Overview of the MW100 Data Acquisition Unit

The MW100 Data Acquisition Unit consists of a main module equipped with an Ethernet port, I/O modules for input and output of signals (these are the same as those for the MX100 Data Acquisition Unit), and a base plate to which the first two items are mounted. The main module comes with a HTTP server function, allowing users to easily enter settings and monitor measured data from a PC using a browser. The MW100 can be used for data acquisition on site as a standalone, enabling data acquisition on up to 360 channels using the Modbus TCP or RTU function.

The MW100 Data Acquisition Unit can be flexibly configured for a variety of measuring environments.

### One-to-one Connection with a PC


This is an example of a system for small scale logging, IP address settings, and other capabilities.

#### Using a browser:

- Easy setting entry
- Monitoring of measured data


#### Using PC software:

- IP address setting
- Calibration

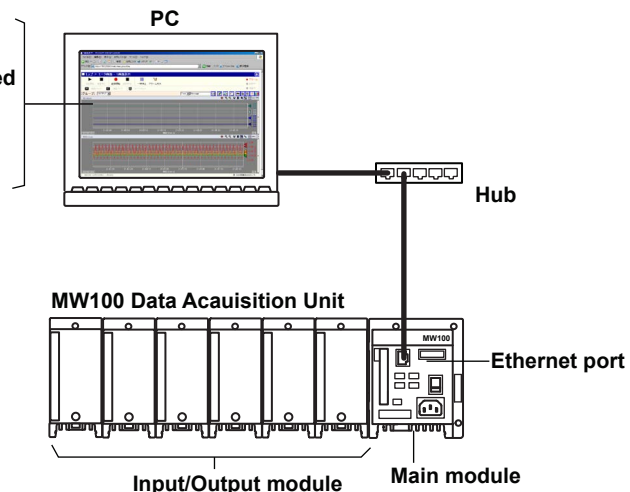

### Standalone Configuration

This is an example of configuration for an on-site standalone data acquisition system.

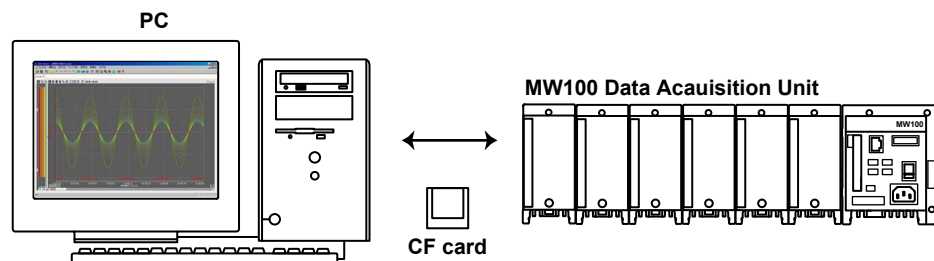

### One-to-N Connection with a PC


Connections can be made via Ethernet or RS-422A/485. For connection examples, see the MW100 Data Acquisition Unit User's Manual (IM MW100-01E).

### Connecting to Modbus Devices

You can connect to Modbus devices. For connection examples, see the MW100 Data Acquisition Unit User's Manual (IM MW100-01E).

## Overview of MW100 Viewer Software


MW100 Viewer Software consists of the three software components described below.

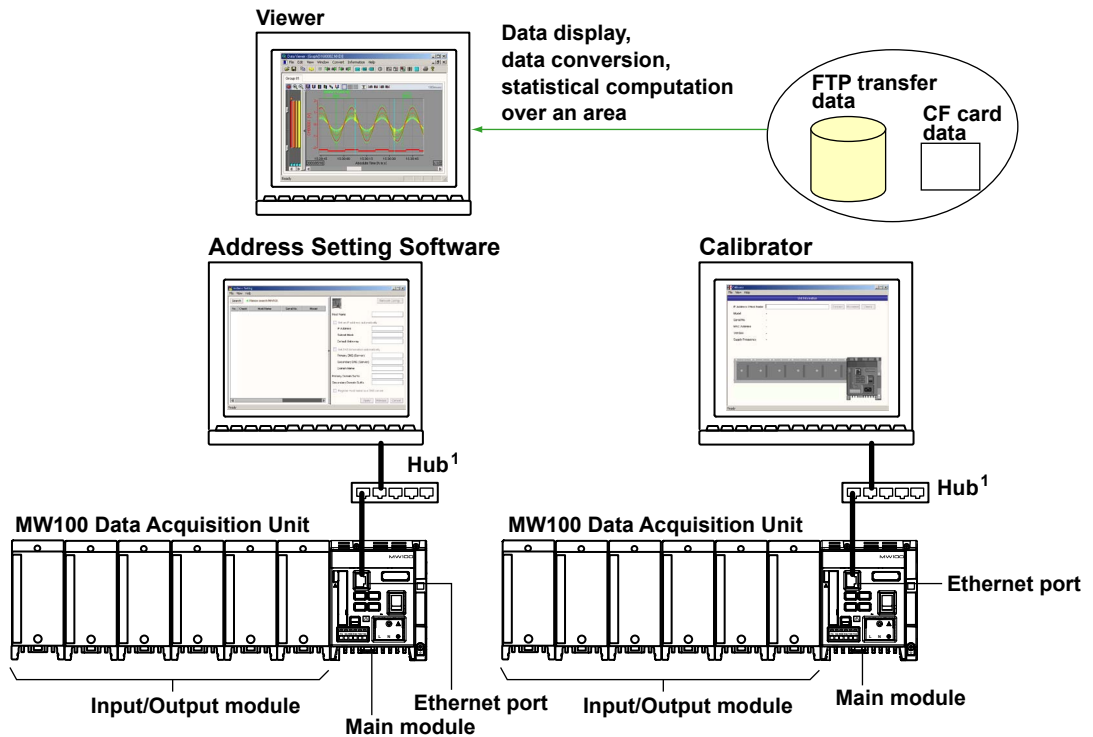

<sup>1</sup> To change the factory default IP address set, open a local (1:1) connection.


## Address Setting Software

The address setting software allows you to enter initial communication settings on the MW100 main unit. The software opens a local (1-to-1) connection with the MW100 main unit, allowing changes to the factory default IP address, and it searches for and displays other MW100s on the same segment. The software allows you to change settings such as the MW100 host name, IP address, DNS server, domain name, and domain suffix, and register a host name on the DNS server.

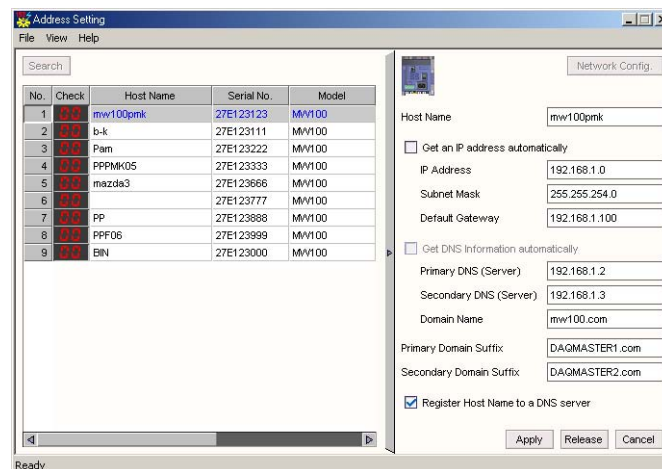

The Address Setting software can also be run directly from the CD-ROM without being installed on the PC. Click a language selection button in the MW100 Viewer Software CD-ROM address setting startup screen.

## Viewer

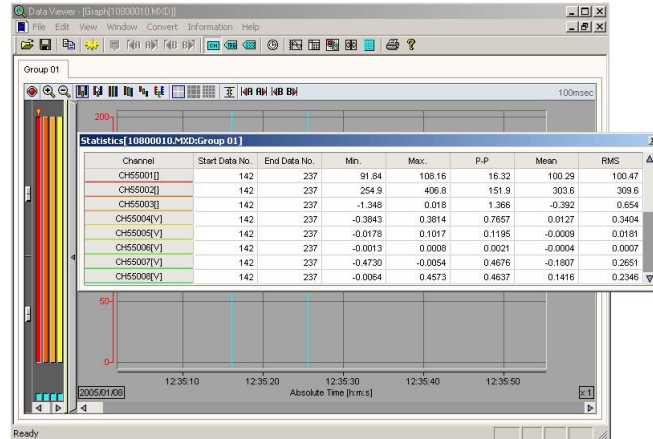

You can load the measured/computed data that was saved in the past and carry out the operations below. You can also display manual sample files and report files.

- Joining  
When opening a divided data file, related files can be joined and displayed.
- Display waveforms and numerical values
- Display the alarm/mark list
- Change the display conditions (group assignments, scale, trip point, display color and other parameters)
- Read data values using the cursor
- Perform statistical computation over an area
- Display and add marks
- Save or load display conditions
- Display the file information
- Convert data formats (ASCII, Excel, and Lotus)
- Print data (waveforms, numeric values, alarm/marker list, cursor values, statistics over an area, and computed values)
- Use and save templates

## Calibrator


This software is used to calibrate the MW100 input/output modules.

You can connect to the MW100, display the modules that can be calibrated, and carry out calibration at each measurement range and output range.



## Flow of Operations during Installation


The figure below shows the general flow of operation when the MX100 is installed initially.

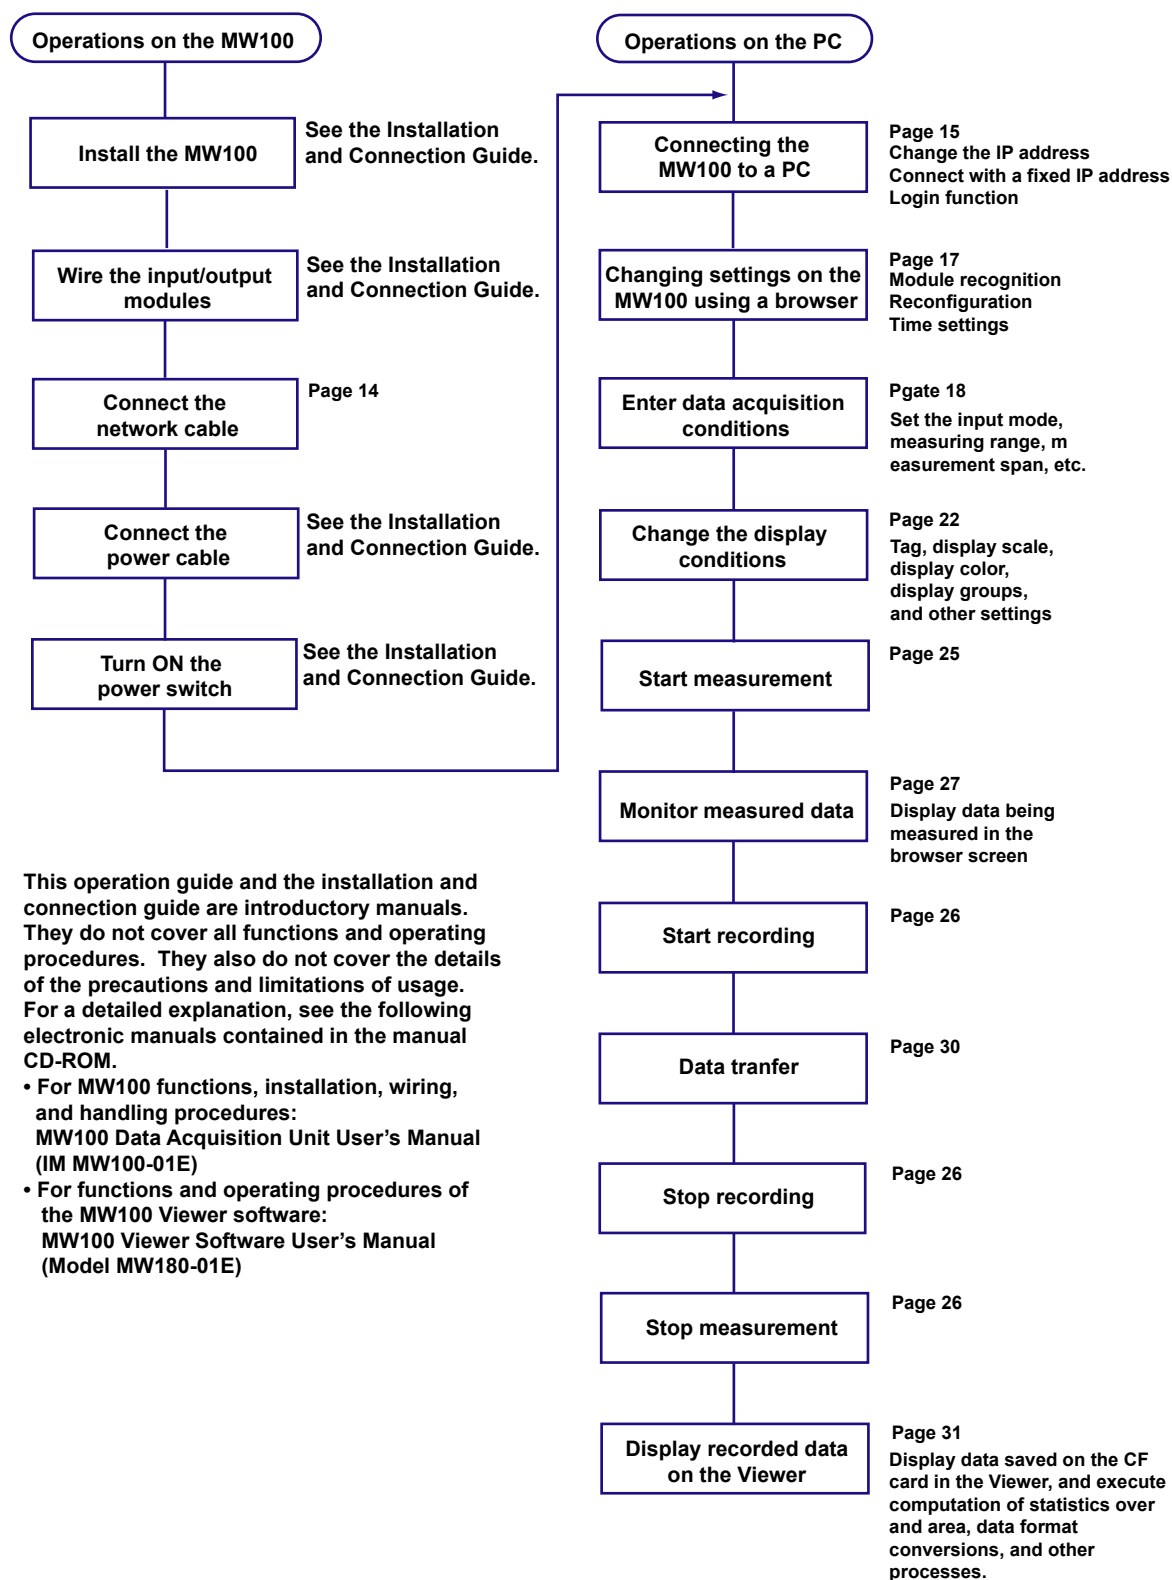

# Connecting to a Network


## Connecting an Ethernet Cable to the Main Module

Connect the Ethernet cable to the Ethernet port on the main module. Use a UTP (category 5 or higher) or STP Ethernet cable.

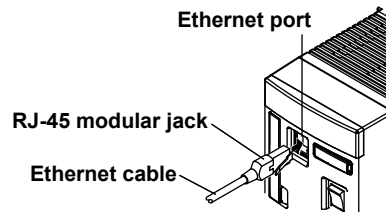


## Checking the Communication Status

You can check the status on the two LEDs at the upper-right and lower-right of the Ethernet port.

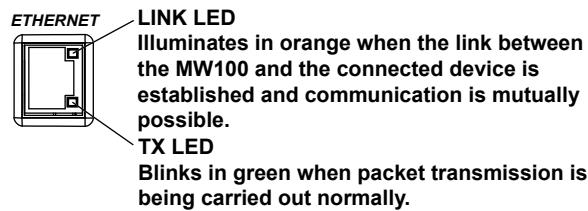

## Connection to the PC

Make the connection via a hub. For a one-to-one connection with a PC, make the connection as shown in the figure below. In the same manner, you can connect multiple MW100 Data Acquisition Units to a single PC.

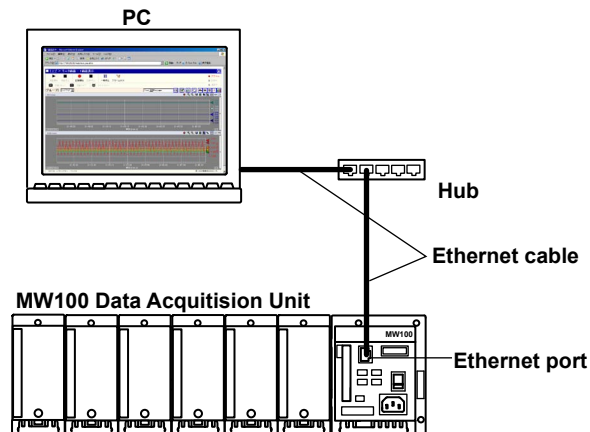


# Connecting the Main Module to a PC

## Ethernet Connection

### Setting the IP Address


Because the IP address is not set by factory default, set the IP address first.

1. After opening an Ethernet connection between the MW100 and PC, run the MW100 Viewer Software CD-ROM or the IP address setting software installed on the PC.
2. Click here.  
The MW100 information is displayed.

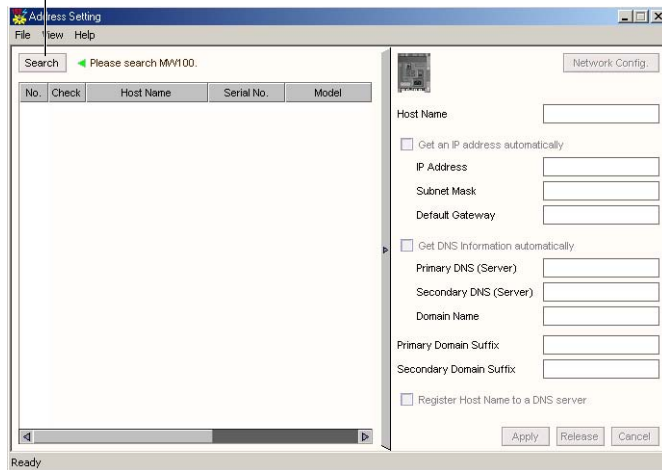

3. Click here.  
Information appears in the address setting screen.

4. Click here.  
Setting changes are enabled.

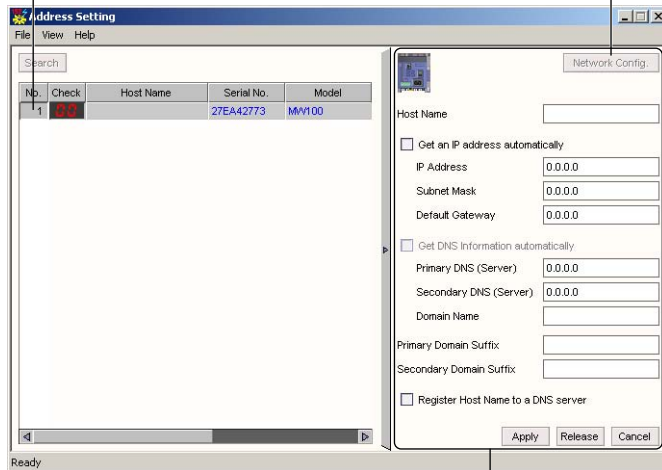


Address Setting Screen

## Connecting the Main Module to a PC

5. Make entries in the address setting screen.  
The following is an example of editing such entries.

Host name: mw100user  
Specify IP address: 192.168.1.100  
Subnet mask: 255.255.255.0  
Default gateway: 192.168.1.1  
Specify a DNS server  
Primary DNS server: 192.168.1.101  
Secondary DNS server: 192.168.1.102  
Specify a domain suffix  
Primary domain suffix: daqmaster1.com  
Secondary domain suffix: daqmaster2.com

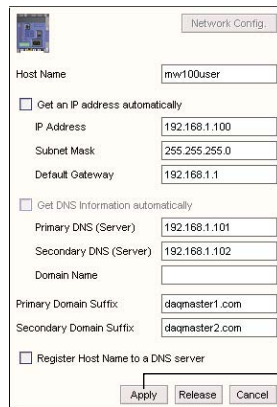

6. Click here.  
The edited items are applied to the MW100.

## Connecting with a Browser

7. Connect an Ethernet cable between the MW100 and PC, then start the browser.
8. Enter the IP address of the MW100 in the browser's URL/Address box.

### Ex. Specifying the IP address using the browser



The MW100 top screen appears. From the browser, you can change MW100 settings, or acquire/record data.



Kind	Status	Operation
Measurement	Stop	▼
MATH	Stop	▼
Recording	Stop	▼



# Entering Settings on the MW100 Using a Browser

## MW100 System Settings

### Display of Module Information and Reconfiguration

1. From the browser top screen, click System Setting > Module Information.  
The module information screen is displayed.

No.	Configured Module	Attached Module	Status
0	MX110-UNV-M10	MX110-UNV-M10	
1	MX110-UNV-M10	MX110-UNV-M10	
2	MX120-PWM-M08	MX120-PWM-M08	
3	MX112-B12-M04	MX112-B12-M04	
4			
5			

2. If the Configured Module and Attached Module displays are different, click here.  
System reconfiguration is executed.  
The Configured Module and Attached Module displays become the same.  
If the attached module does not appear, turn OFF the power and check that the module is attached correctly.

### Setting the Date and Time

3. After choosing System Setting in step 2, click Date and Time Setting.  
The date/time setting screen appears.

Date year: 5 month: 1 day: 1

Time 11 : 20 : 56

Time Zone 9 : 0

Apply

4. Change the date and time setting.  
The following is an example.  
Date: October 25, 2007  
Time: 10:25:00  
Time zone: 9:00.

Date year: 07 month: 10 day: 25

Time 10 : 25 : 0

Time Zone 9 : 0

Apply

Enter the last two digits of the Western calendar.

This differs depending on the country and region.  
For Japan, it is 9:00.

5. Click here.  
The date and time settings are changed.

**Checking Free Space on the CF Card and Initializing**

- After choosing System Setting in step 5, click System Information. The amount of free space on the CF card is shown under Media Information.

**Top > System Setting > System Information**

System Information

Model: MW100

Serial No.: 77EA77777

Option: MATH DEG\_F RS-422 DST

Version: R3.01

Web Version: R3.01

Initializing Level: [dropdown]

Media Information

Capacity: 494352 / 500176 K byte free

Format: [Execute]

Initialize [button]

- To initialize the CF card, click here, then click the Initialize button.

**Measurement Groups and Measurement Module Settings**

- From the browser top screen, click System Setting > Measurement Setting. The measurement operation setting screen is displayed.

**Top > System Setting > Measurement Setting**

Interval Group

No.	Interval
1	100 ms
2	500 ms
3	1 s

Measurement Module

Module No.	Interval Group	A/D Integration Time
0	1	Auto
1	2	50 Hz
3	3	50 Hz
1		
1		

Apply [button]

- Click to select the measuring interval.
- Click to select measurement groups of the measurement intervals above for the input modules.
- Click here, then select the integral time from the list.
- If an output module is connected, or if a module is not connected, it is not displayed.
- Click here. The settings are changed.

**Note**

- The Interval Group that is assigned to the measurement group number is set as: (interval is short) Interval group1 ≤ Interval group2 ≤ Interval group 3 (interval is long)
- The equivalent of three modules worth of settings are entered for the 30-CH Medium Speed DCV/TC/DI Input Module.
  - Select the same measurement group for the three measurement groups.
  - Select the same integral time for the three A/D integral times.

## Settings for Recording to CF Card

1. From the browser top screen, click System Setting > Recording Setting.  
The recording operation setting screen is displayed.

2. Click here, then select the save start operation.

3. Click here to select the type of recording.

Top > System Setting > Recording Setting

No.	Mode	Action	Recording Interval	Data Length	Pre-trigger
1	Direct	Rotate	1		
2	Direct	Full Stop	2		
3	Trigger	Single	1	10 min	0 %

4. Click to select the recording interval.  
Set an integer multiple of the measurement interval.

6. Select a trigger length if data is to be saved upon activation of the trigger.  
Specify a pretrigger length as a percentage of the data length.

Recording Action

DIRECT Data Length

30 min

Limit for Media Alarm

1 h

5. Select the data length.

7. Click to select the time remaining for activating the media alarm.

8. Click here.  
The settings are changed.

Apply

## Recording Channel Settings

1. From the browser top screen, click Channel Setting > Recording Channel Setting.  
The recording channel setup screen appears.

Top > Channel Setting > Recording Channel Setting

Channel List 001 - 010

No.	Record	Thinning Record	Manual Sample
001	On	On	On
002	On	On	On
003	On	On	On
004	On	On	On
005	On	On	On
006	On	On	On
007	On	On	On
008	On	On	On
009	On	On	On
010	On	On	On

2. Click here to select the recording channel range.

For information on thinning recording and Manual Sample, see the MW100 Data Acquisition Unit User's Manual (IM MW100-01E). Thinning recording (section 3.4), Manual Sample (section 1.3)

3. Click here to select to record (On) or not to record (Off).

4. Click here.  
The settings are changed.

Apply

## Measuring Interval and Range Settings (for the Universal Input Module)

1. From the browser top screen, click Channel Setting > AI/DI Channel Setting. The input range setting screen appears.
2. Click the list, then select the channel range you wish to set.

Top > Channel Setting > AI/DI Channel Setting

Channel List: 001 - 010

No.	Mode	Range	Span		Calc	Ref Ch.	Scale			Unit
			Lower	Upper			D.P.	Lower	Upper	
001	VOLT	2V	-2.0000	2.0000	Off					
002	VOLT	2V	-2.0000	2.0000	Off					
003	VOLT	2V	-2.0000	2.0000	Off					
004	VOLT	2V	-2.0000	2.0000	Off					
005	VOLT	2V	-2.0000	2.0000	Off					
006	VOLT	2V	-2.0000	2.0000	Off					
007	VOLT	2V	-2.0000	2.0000	Off					
008	VOLT	2V	-2.0000	2.0000	Off					
009	VOLT	2V	-2.0000	2.0000	Off					
010	VOLT	2V	-2.0000	2.0000	Off					

Apply

Global Setting

No.	Mode	Range	Span		Calc	Ref Ch.	Scale			Unit
			Lower	Upper			D.P.	Lower	Upper	
001	VOLT	2V	-2.0000	2.0000	Off					
010										

Apply

3. Set the input type, measuring range, measurement span, scale, and other items. The following is an example. For procedures for setting up an input module other than the universal input module, see the MW100 Data Acquisition Unit's user's manual (IM MW100-01E), chapter 3.

Top > Channel Setting > AI/DI Channel Setting

Channel List: 001 - 010

No.	Mode	Range	Span		Calc	Ref Ch.	Scale			Unit
			Lower	Upper			D.P.	Lower	Upper	
001	VOLT	2V	-2.0000	2.0000	Off					
002	TC	R	0.0	1760.0	Off					
003	RTD	Pt100-1	-200.0	600.0	Off					
004	DI	LEVEL	0	1	Off					
005	FRJC	R	0.0	1760.0		001				
006	VOLT	2V	-2.0000	2.0000	Scale		1	0.0	1000.0	kg
007	VOLT	6V	-6.000	6.000	Scale		0	-30000	30000	kV
008	VOLT	2V	-2.0000	2.0000	Off					
009	VOLT	2V	-2.0000	2.0000	Off					
010	VOLT	2V	-2.0000	2.0000	Off					

Apply

Global Setting

No.	Mode	Range	Span		Calc	Ref Ch.	Scale			Unit
			Lower	Upper			D.P.	Lower	Upper	
001	VOLT	2V	-2.0000	2.0000	Off					
010										

Apply

4. Click here. The range is changed.

## Alarm and Relay Settings

- From the browser top screen, click Channel Setting > Alarm Setting (AI/DI).  
The alarm setting screen is displayed.

Top > Channel Setting > Alarm Setting (AI/DI)

Channel List: 001 - 005

No.	Alarm			Output		
	No.	Type	Value	Hysteresis	Action	Relay
001	1	Off				
	2	Off				
	3	Off				
	4	Off				
002	1	Off				
	2	Off				

- Select the channel range you wish to set in the list.

- Select the alarm type, then enter the alarm value and hysteresis.  
For details on alarm setting items, see the MW100 Data Acquisition Unit User's Manual (IM MW100-01E), section 1.3.

Top > Channel Setting > Alarm Setting (AI/DI)

Channel List: 001 - 005

No.	Alarm			Hysteresis	Output	
	No.	Type	Value		Action	Relay
001	1	H	1.0000	0.0000	On	021
	2	L	-1.0000	0.0000	On	022
	3	Off				
	4	Off				
002	1	L	2.0000	0.0000	On	030
	2	Off				
005	1	Off				
	2	Off				
	3	Off				
	4	Off				

- Apply
- Click here.  
The alarm settings are changed.

- After choosing Channel Setting in step 4, click DO Channel Setting.  
The relay setting screen is displayed. For details, see the MW100 Data Acquisition Unit User's Manual (IM MW100-01E), sections 3.7 and 3.8.

Top > Channel Setting > DO Channel Setting

Channel List: 021 - 030

No.	Kind	Energize	Hold	Action	Refresh
021	Alarm	Energize	Off	And	
022	Alarm	Energize	Off	And	
023	Alarm	De-energize	Off	Or	On
024	Alarm	Energize	On	Or	
025	Alarm	De-energize	Off	Or	Off
026	Comm. Input	Energize			
027	Comm. Input	Energize			
028	Media				
029	Fail				
030	Error				

Apply

- Click the channel range for which you wish to set relays.

- Enter or select each item.  
For details on relays, see the MW100 Data Acquisition Unit User's Manual (IM MW100-01E), section 1.12.

- Click here.  
The relay settings are changed.

# Changing Monitor Screen Display Conditions

Stop measurement, then change the display method.

After changing the display method, start measurement and display the monitor screen.

The screen is updated according to the new settings. For details on display settings, see the MW100 Data Acquisition Unit User's Manual (IM MW100-01E), section 3.15.

## Tag Settings

1. From the browser top screen, choose Display Setting > Channel Tag Setting. The tag setting screen is displayed.

Top > Display Setting > Channel Tag Setting

Channel List 001-010


No.	Tag Name
001	ROOM1
002	ROOM2
003	ROOM3
004	FLOOR1
005	FLOOR2
006	FLOOR3
007	ENTRANCE
008	KITCHEN
009	BATH
010	TOILET

Apply

2. Click here to select the setting range for the tags you wish to set.

3. Enter the tag name. (If no name is entered, the channel number is displayed.)

Tag name (Channel number)



4. Click here. The tag name setting is changed.

5. After choosing Display Setting in step 4, click Other Settings.

Top > Display Setting > Other Settings

Channel No./Tag Display

Tag Name

Apply

6. Click here to select the Tag Name.

7. Click here.

## Setting Messages

1. From the browser top screen, choose Display Setting > Message Setting. The message setting screen is displayed.

Top > Display Setting > Message Setting

Message List

No.	Message
1	Message01
2	Message02
3	Message03
4	Message04
5	Message05


Apply

2. Enter a message.

3. Click here. The message setting is changed.

### Operation in the browser's monitor screen


1. Select a message (Free, or 1 to 5).
2. If you select Free, enter characters (up to 15 alphanumeric).

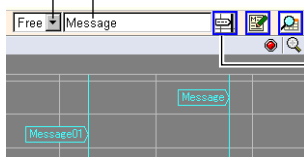

3. Click here. The selected message is displayed on the monitor screen.

## Display Scale Settings

- From the browser top screen, choose Display Settings > Graph Scale Setting. The scale setting screen is displayed.

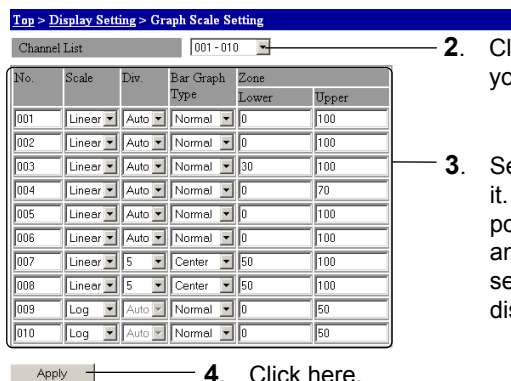


- Click to select the channel range you wish to set.

- Select each setting item, or specify it. The graph display reference position is applied to the numerical and bar graph displays. Other settings are applied to all types of display screens.


- Click here. The display settings are changed.

### Scale Setting Example

Linear  
(no. of scale divisions can be selected)




Log  
(no. of scale divisions: fixed to Auto)




### Scale division setting example


From the top, 1, 2, 3, or 4 divisions



### Graph display position setting example

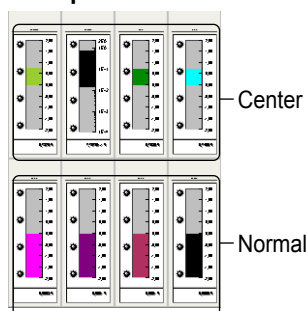


### Zone Setting Example

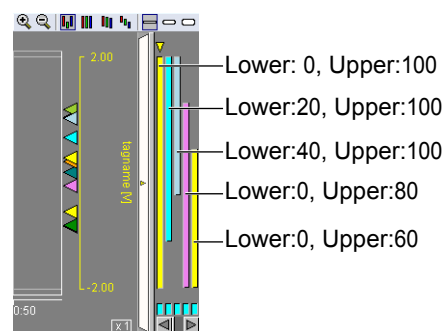

### Display Color Settings


1. From the browser top screen, choose Display Setting > Channel Color Setting. The color setting screen is displayed.

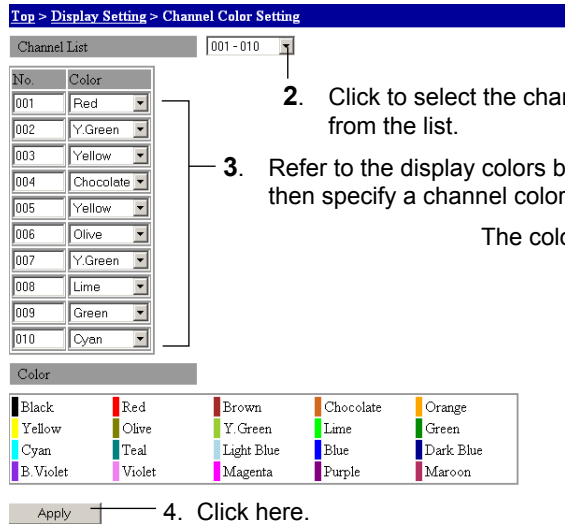

2. Click to select the channel range you wish to set from the list.

3. Refer to the display colors below, then specify a channel color.


The color changes to the one specified.

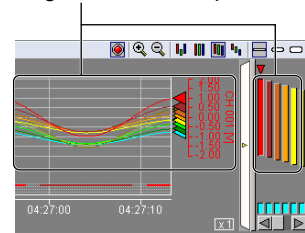

4. Click here. The color settings are changed.

### Display Group Settings

1. From the browser top screen, choose Display Setting > Display Group Setting. The display group setting screen is displayed.

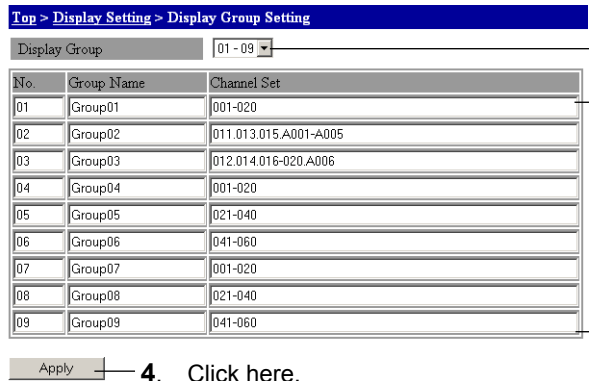


2. Click to select the display group range you wish to set from the list.

3. Enter group names and channels to include. You can specify a group name using up to fifteen alphanumeric characters. Up to twenty display channels can be registered to a single group. Individual channel numbers are delimited with periods ( . ), and ranges of channels can be specified with hyphens. The following is an example of a channel specification.

001.003.005 (001, and 003, and 005)  
 004-008 (004 through 008)  
 001.A001-A005 (001, and A001 through A005)

4. Click here. The group settings are changed.

Click here. The set group names are displayed in the list. Select the group you wish to display. The measured data of the channels specified for the group is displayed.

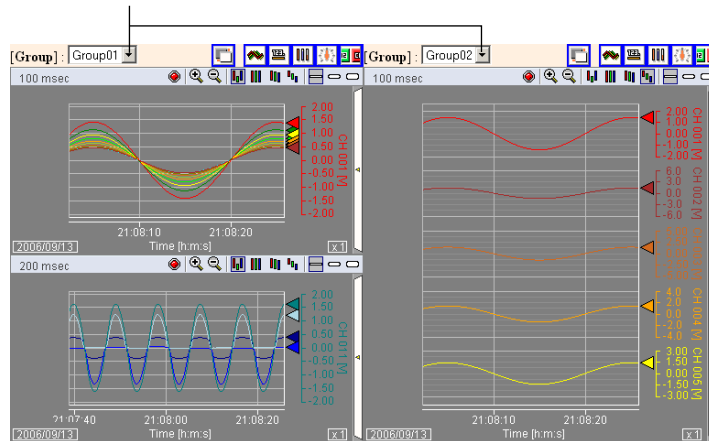





# Starting and Stopping Measurement and Recording

To start and stop measurement and recording, you can use the keys on the MW100 Main Module, or use the browser.

## • Using the Keys

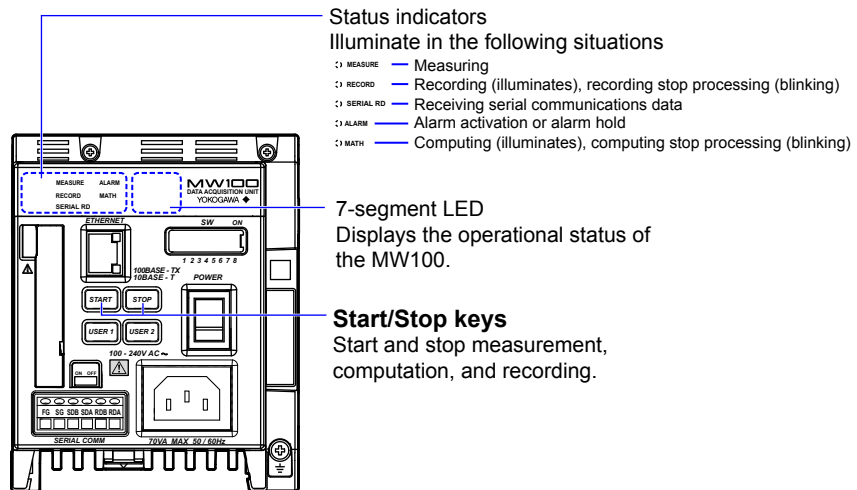

## • Using a Browser

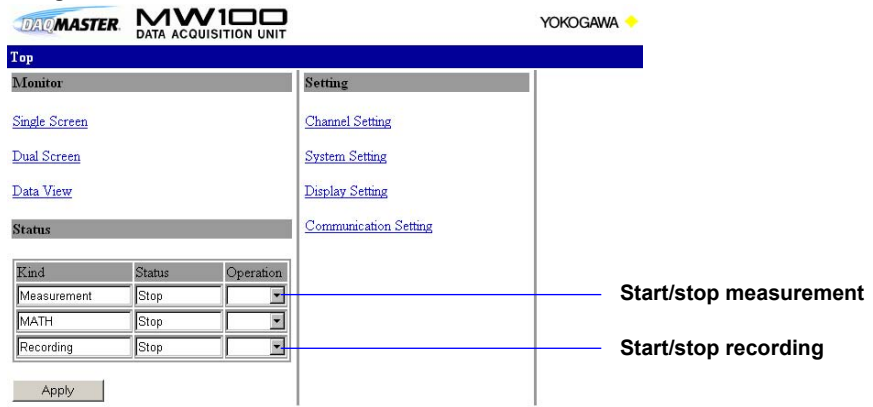

## Starting Measurement

1. Check whether the instrument is measuring or recording by looking at the MW100 main module's status lamp, or the browser's top screen.
2. Briefly press the MW100 main module's START key, or select Start in the Operation list under Measurement in the browser top screen's Status table. Measurement begins.

### Starting Recording

1. Check whether the instrument is measuring by looking at the MW100 main module's status indicator, or in the browser's top screen.
2. Press the MW100 main module's START key for about two seconds, or select Start in the Operation list under Recording in the browser top screen's Status table.

Measured data is saved to the CF card.

File menus are automatically generated using the date and serial number.

**MDDIXXX.MXD**

- M: Month file created (local time), 1 to 9, X (October), Y (November), Z (December)
- DD: Date when file created (local time), 1 to 31
- I: Files in measurement groups 1 to 3 are 1 to 3  
Computed data file is M  
Thinned values, T
- XXXX: Sequence number 0000 to 9999
- MXD: MW100 file extension (uppercase)

### Stopping Recording

1. Check whether the instrument is measuring or recording by looking at the MW100 main module's status indicator, or the browser's top screen.
2. Press the MW100 main module's STOP key for about two seconds, or select Stop in the Operation list under Recording in the browser top screen's Status table.  
Recording stops.


### Stopping Measurement

1. Check whether the instrument is measuring or stopping recording by looking at the MW100 main module's status indicator, or the browser's top screen.
2. Briefly press the MW100 main module's STOP key, or select Stop in the Operation list under Measurement in the browser top screen's Status table.  
Measurement stops.

**Note**

This document does not cover MATH settings, or how to start and stop computation. Please refer to the *MW100 Data Acquisition Unit user's manual* (IM MW100-01E).


The process is described in the status transition diagram.

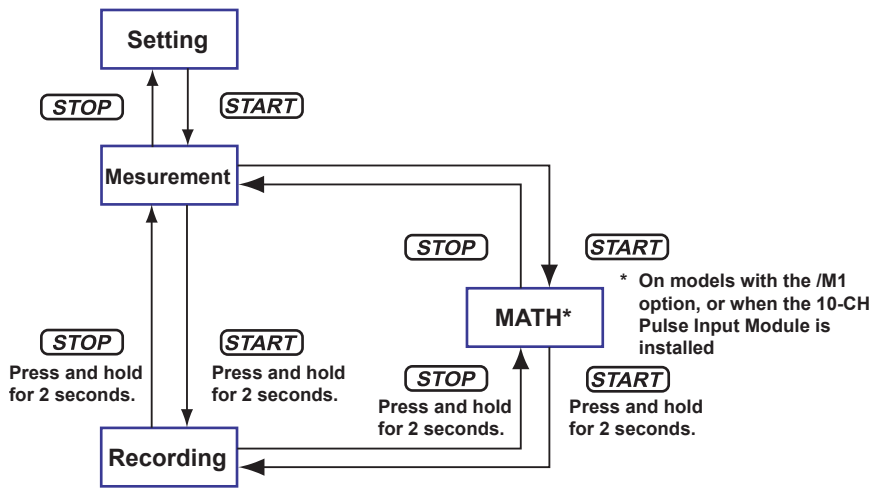

# Viewing Measured Data on the Monitor Screen and Starting/Stopping Recording

In the browser monitor screen, you can view data being measured in a trend, numerical, meter, or bar graph display. You can also start and stop recording, pause the monitor display, write messages, and perform other functions.

1. Check whether the instrument is measuring by looking at the MW100 main module's status indicator, or in the browser's top screen.
2. From the browser top screen, click Single Screen or Dual Screen.

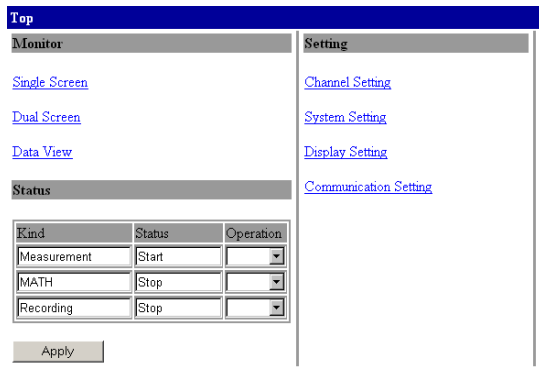

The Measured data screen appears.

## Single Screen (Trend Display)

**Computation start/stop button**  
Starts and stops computation (with the /M1 option, or when the 10-CH Pulse Input Module is installed).

**Recording Start/Stop button**  
Starts and stops data acquisition.

**Pause button**  
Pauses monitor display updating. Data acquisition does not stop.

**Alarm ACK button**  
If set to hold alarms, alarms are cleared upon alarm clear wait. (Includes relay action)

**Output channel operation icons (When output modules installed)**  
Area for displaying manual DO and operation icons for arbitrary output. Displays one channel's worth.


**Operational status**  
Illuminates during alarms, recording, and computation.

**Switch operation icon**  
Switches the size of the icon.


**Viewing Measured Data on the Monitor Screen and Starting/Stopping Recording**

**Dual Screen (Trend Display)**

Use this when the monitor screen contains two screens. You can display two groups. From the top screen, click Dual Screens.

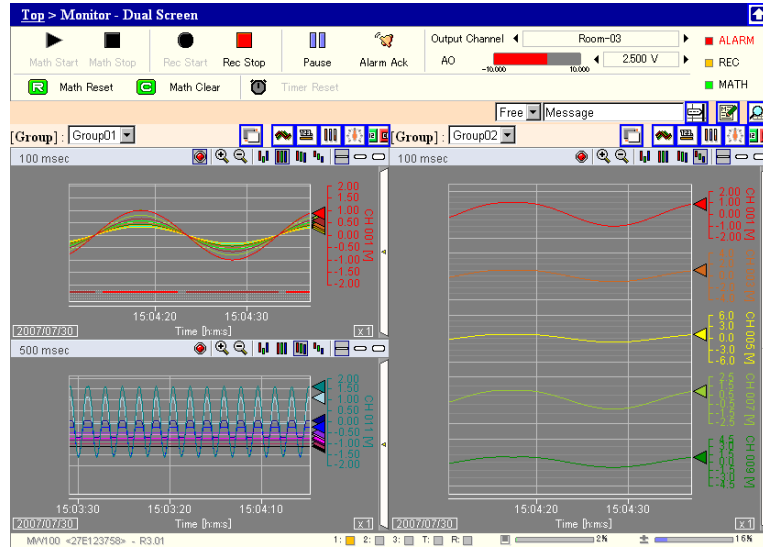

The contents of the status bar are as follows:

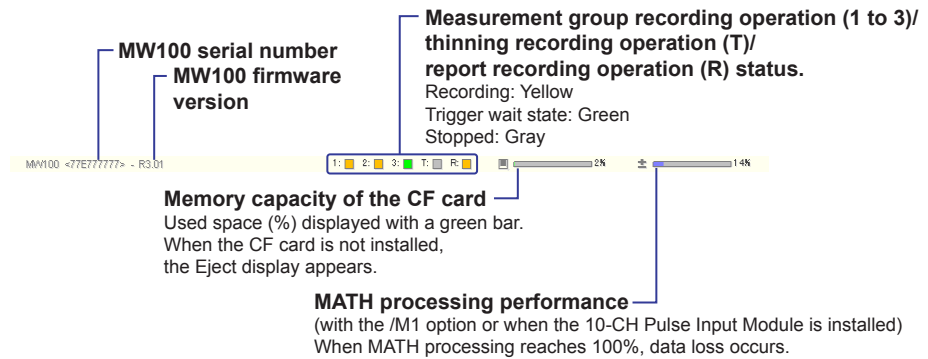


**Switching the Display Group and Monitor Display**

3. To change the displayed group, select a group in the Select Display Group list in the figure below.

To switch the monitor display, click the Select Monitor Display button in the figure below.


The screen display switches.

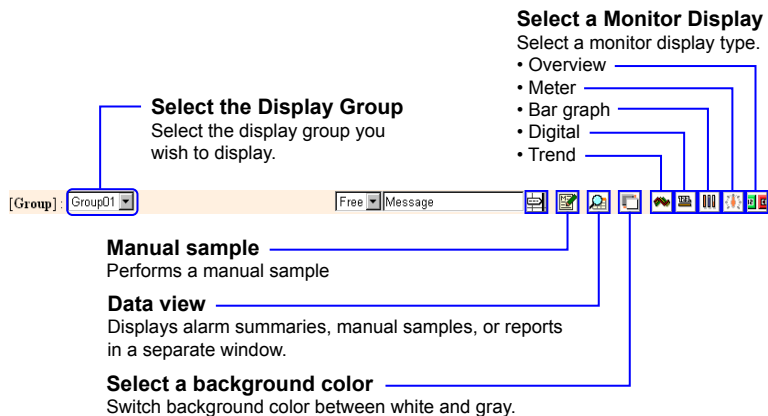

## Viewing Measured Data on the Monitor Screen and Starting/Stopping Recording

### • Digital Display

Displays measured values as numerical values. When alarms are set, the alarm status is displayed to the left of the numerical value.

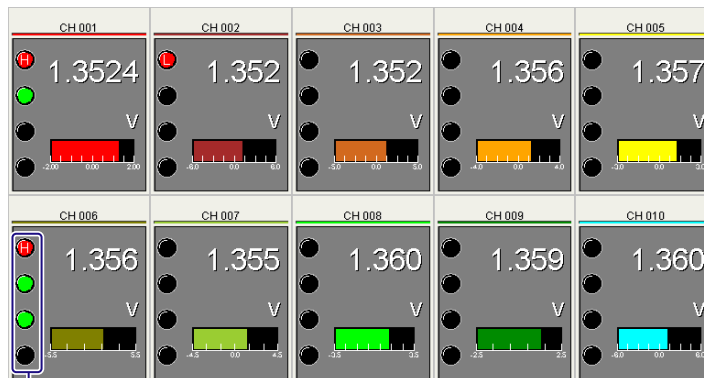


#### Alarm status

Black ● Alarm not set up  
 Green ● Illuminated: No alarm occurring  
 Blinking: Alarm hold clear wait after alarm factor cleared  
 Red ● Illuminated: Alarm occurring  
 (symbol in circle is alarm type: H/L/rH/rL/dH/dL/tH/tL)  
 Blinking: Alarm hold clear wait after alarm factor occurrence


### • Bar Graphs

Displays measured values in a bar graph. When alarms are set, the alarm status is displayed to the left of the bar graph. For information on alarm statuses, see Digital Display.

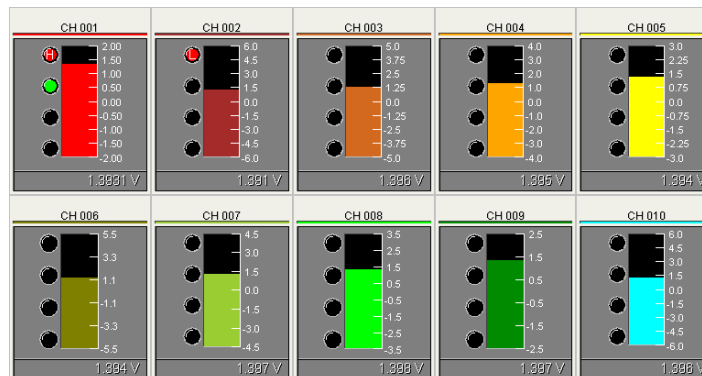

### • Meters

Displays measured values in a meter. When alarms are set, the alarm status is displayed to the left of the meter. For information on alarm statuses, see Digital Display.

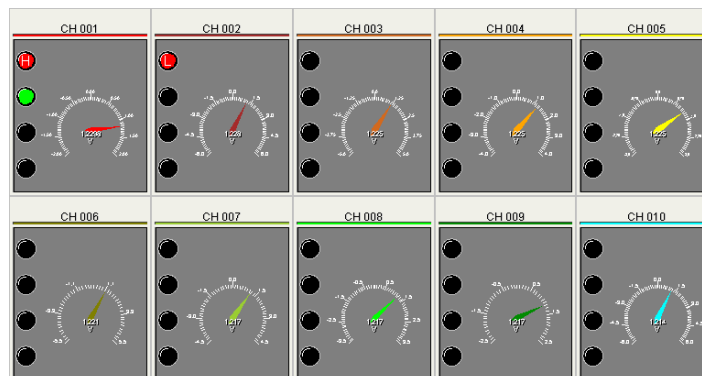

## Viewing Measured Data on the Monitor Screen and Starting/Stopping Recording


### • Overview Display

Alarms (status and type) and measured values are displayed as numerical values in the monitor display screen. Skipped channels are not displayed. If the size of the window is reduced, only the alarms are displayed.

CH 001 0.5792 v	CH 002 0.5189 v	CH 003 0.4593 v	CH 004 H 0.3996 v
CH 005 0.0019 v	CH 006 H 1.2325 v	CH 007 0.8302 v	CH 008 L 0.0052 v
CH 009 0.3668 v	CH 010 0.0013 v	CH 011 0.0000 v	CH 012 0.0000 v
CH 013 0.0000 v	CH 014 0.0000 v		


### Starting Recording

- Click the Record Start button in the screen display.  
Saving of data to the CF card begins.



### Stopping Recording

- Click the Record Stop button in the screen display.



## Transferring Measured Data to the FTP Server

- From the browser top screen, choose Communication Setting > FTP Client Setting. The FTP client settings screen opens.

Top > Communication Setting > FTP Client Setting

FTP Client Function	<input checked="" type="checkbox"/> Enable
Time Shift	0 min
FTP Server	1
Server	ftp.daqmaster.com
Port	21
User	mw100user
Password	<input checked="" type="checkbox"/> [REDACTED]
Directory	/data
PASV Mode	<input type="checkbox"/> Enable
Apply	

- Set the items such as the FTP server name.


- Click here. The settings are changed.


- Start the measurement and then start the recording. (For the procedure to start the measurement and recording, see pages 20 to 22 in this manual.)  
When a file is created, the file is transferred to the folder on the specified FTP server.

# Viewing Measured Data on the Viewer Software

## Displaying Data

You can view data files saved to the CF card and data files that have been transferred to the PC from the FTP server using the Viewer.

1. Choose Programs > MW100 Viewer > MW100 Viewer to start the Viewer.
2. Click the  button on the toolbar or choose Open from the File menu. The Open dialog box opens.

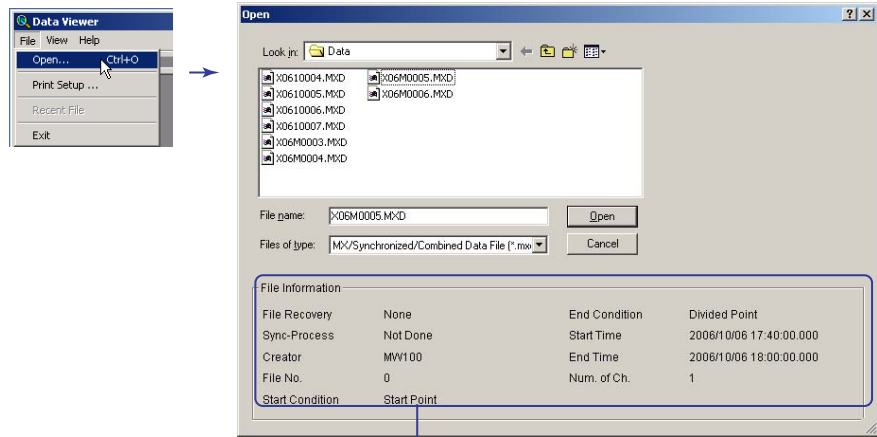

File information


3. Select the file you wish to load and click the Open button. The waveform display window opens.

### When Loading Divided Data Files on the MW100

Before the waveform display window is displayed, if a file that can be joined exists, a dialog box opens with the message "Combining with related files?" To join the data files, click Yes. To display only the specified file, click No.




Opens the waveform display window

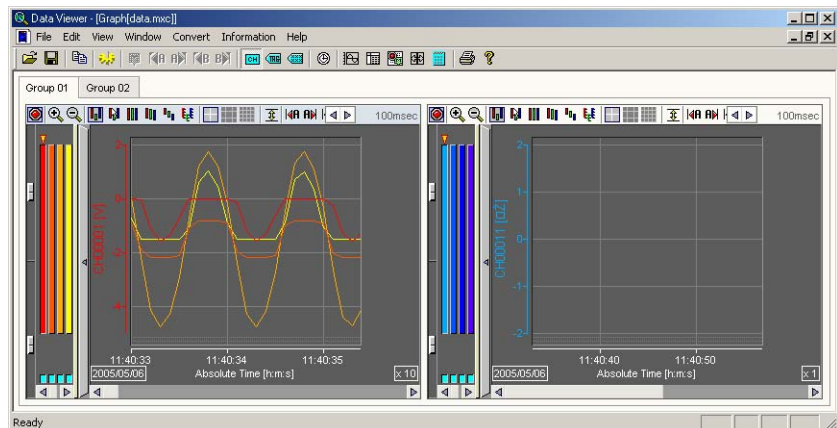

Files are divided into the graphs and math channel graphs at the recording interval specified on the browser even when in the same group.


### Changing the Display on the Waveform Display Window

Change the display settings according to the explanation in the figure below.

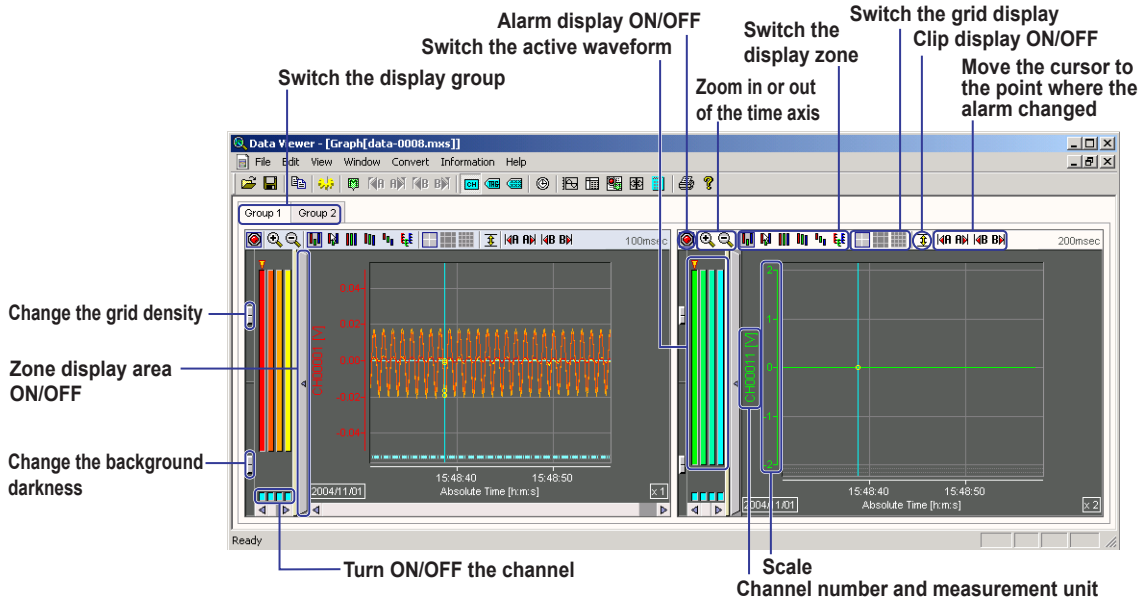


### Changing the Display Using the Toolbar

Change the display settings according to the explanation in the figure below.

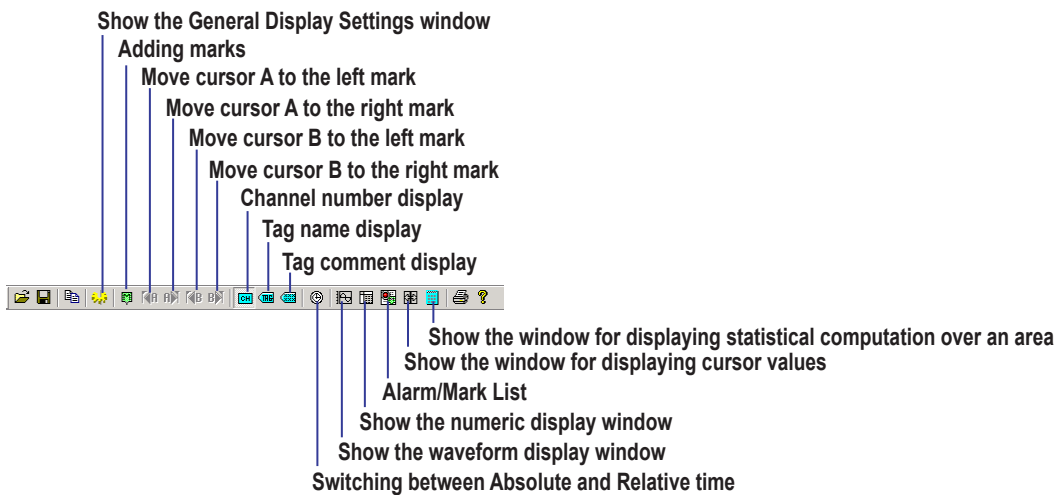

### Changing the Display Using the Menu


You can display the Edit, View, and Window menus.

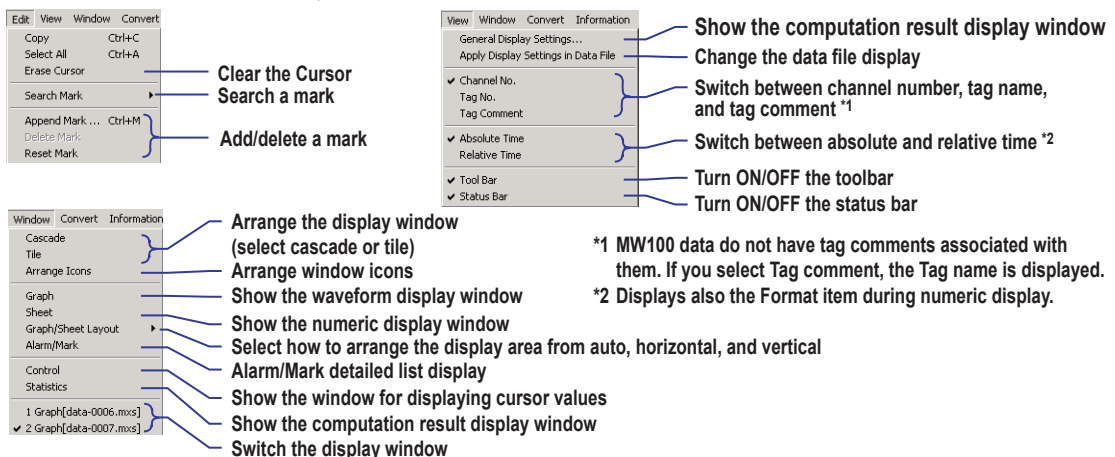




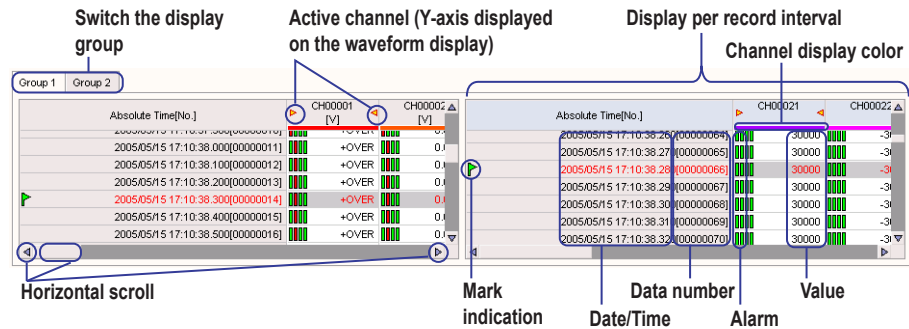
### Changing the Display Using the Display Setup Window

See the explanation in the figure below. Change the display settings and click OK. Set the display for each display group.

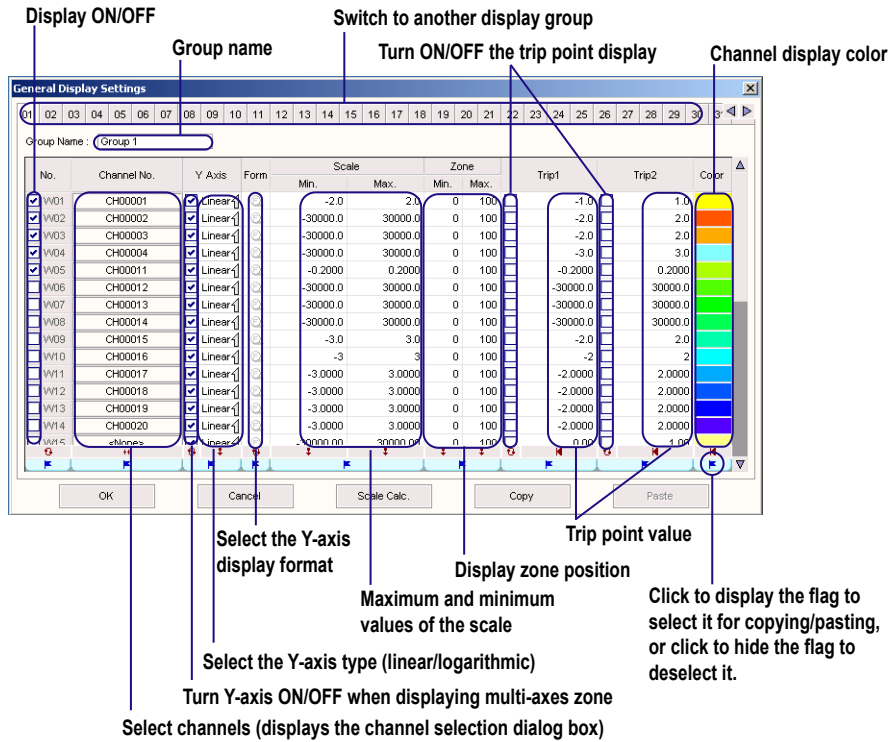


### Numerical Display

While the waveform display window is displayed, click the  button on the toolbar or select Window > Numerical Display to display a numerical value window as in the figure below. If there are groups with differing monitor intervals, the screen is split.




## Reading Values Using the Cursor

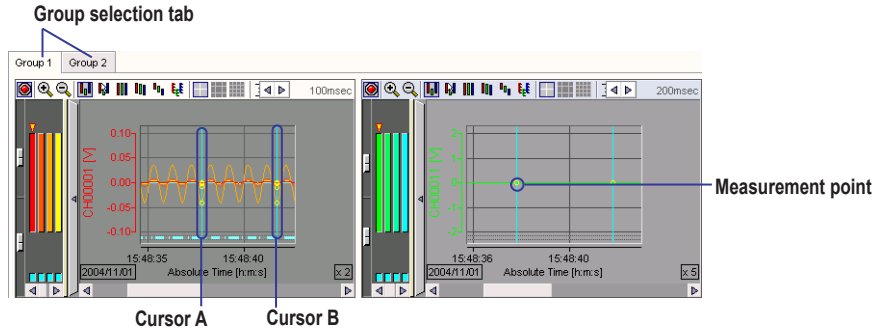


- Click the mouse where you wish to read the data in the waveform display window. If you wish to read another point simultaneously, drag the cursor. Cursor A appears at the position where you first clicked; Cursor B appears at the position where you released the mouse button.

- From the Window menu, choose Cursor value display. The Cursor window opens as shown in the figure on the right.

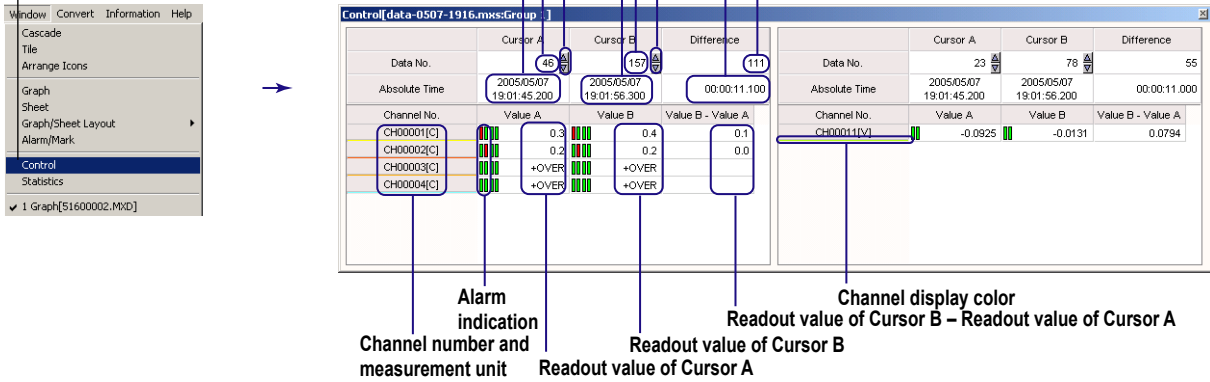

## Statistical Computation over an Area of Measured/Computed Data

- In the waveform display window, click the tab of the group on which you wish to perform statistical computation over an area.
- Click the start position of the computation area in the waveform display area. A light-blue cursor appears in the waveform display area. If multiple waveform display areas are displayed, the cursor is displayed at the time position each waveform display area.
- Drag the cursor to the end position of the computation area. Another light-blue cursor appears at the position where the cursor was dragged.

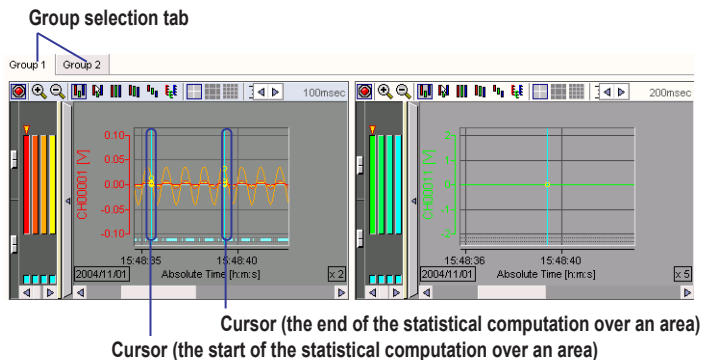

- From the Window menu, choose Statistics.  
The Statistics window opens.

Channel display color

Data number at the start position of the statistical computation over an area

Minimum value

Maximum value - Minimum value

RMS value

Channel number and measurement unit

Data number at the end position of the statistical computation over an area


Maximum Value

Average value

Scroll the channel

Channel No.	Start Data No.	End Data No.	Min.	Max.	P-P	Mean	RMS
CH00001[C]	46	57	0.3	0.3	0.2	0.3	0.3
CH00002[C]	46	57	0.2	0.3	0.1	0.2	0.2
CH00003[C]	46	57					
CH00004[C]	46	57					
CH00011[V]	23	78	-0.0925	-0.0131	0.0794	-0.0345	0.0425
CH00012[C]	23	78					
CH00013[C]	23	78					
CH00014[C]	23	78					

### Alarm/Mark List

- Click the button  on the toolbar or choose Alarm/Marker List from the Window menu.
- Alarm List Display

Sorted according to the clicked item

Currently sorted to the item indicated by this mark

Tag No.	Level	Type	Alarm ON	Alarm OFF
	2	Low	2005/01/05 10:03:04.500	2005/01/05 10:03:07.500
	1	High	2005/01/05 10:03:08.000	2005/01/05 10:03:12.000
	2	Low	2005/01/05 10:03:12.500	2005/01/05 10:03:16.500
	1	High	2005/01/05 10:03:17.000	2005/01/05 10:03:21.000
	2	Low	2005/01/05 10:03:21.500	2005/01/05 10:03:26.000
	1	High	2005/01/05 10:03:26.500	2005/01/05 10:03:30.500
	2	Low	2005/01/05 10:03:31.000	2005/01/05 10:03:35.000
	1	High	2005/01/05 10:03:35.500	2005/01/05 10:03:40.000
	2	Low	2005/01/05 10:03:40.500	2005/01/05 10:03:44.500
	1	High	2005/01/05 10:03:45.000	2005/01/05 10:03:49.000

- Mark List Display

Sorted according to the clicked item

Currently sorted to the item indicated by this mark

Absolute Time	Mark	Group	Marker	Kind
2005/01/05 10:03:20.000	CAUTION			Mark
2005/01/05 10:03:37.500	Mark			Mark
2005/01/05 10:03:46.000	CHECK			Mark
2005/01/05 10:04:01.500	Mark			Mark
2005/01/05 10:04:17.500	BREAK			Mark
2005/01/05 10:04:36.000	Mark			Mark
2005/01/05 10:05:16.000	CHECK			Mark
2005/01/05 10:05:52.000	Trigger Point			Trigger

Message mark added in the browser display screen


Mark added by Viewer software

MW100 trigger marks

Names of groups with marks  
If the groups have no names, all groups are marked

## Setting the Contents to Be Printed

1. From the File menu, choose Print Settings.  
The Print Settings dialog box in the figure below opens.
2. Edit the print settings.

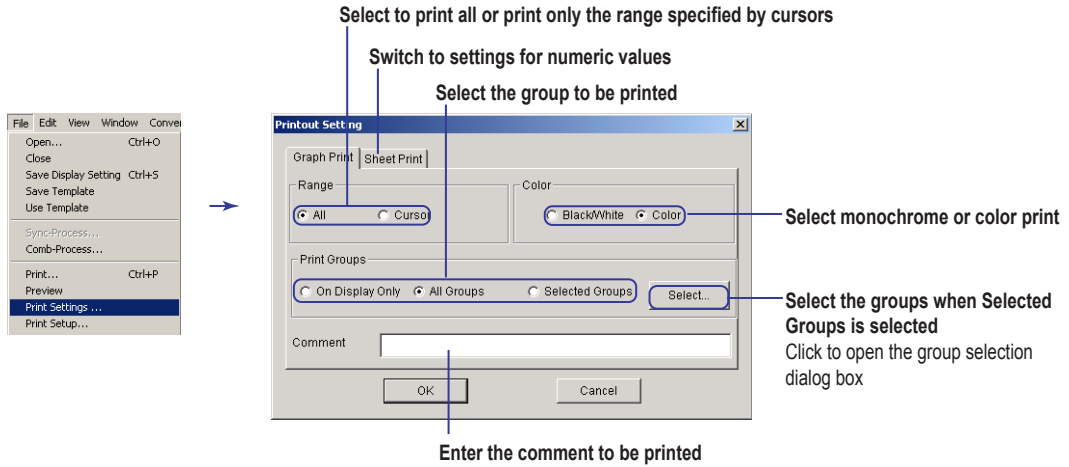

## Converting Data Formats

The data formats below can be changed.

ASCII	Text data with each data point separated by a comma. The extension is .txt.
Excel	Data that can be opened using Microsoft's spreadsheet application Excel version 4.0 or later. The extension is .xls.
Lotus	Data that can be opened using IBM's Lotus 1-2-3 spreadsheet application version 2.0 or later. The extension is .wj2.

From the Convert menu, choose ASCII, Excel, or Lotus, then execute the conversion in the dialog box that is displayed as shown in the figure below. There is a limit to the number of data points that Excel and Lotus1-2-3 can handle. Before executing the conversion, set the channels/groups to be converted, the conversion range, and the step so that the number of data points is appropriate.

