

# Rational Conversion of Affinity Reagents into Label-Free Sensors for Peptide Motifs by Designed Allostery

Jin Huang and Shohei Koide\*

Department of Biochemistry and Molecular Biology, The University of Chicago, Chicago, Illinois 60637

**B**iosensors exploiting molecular recognition by proteins and nucleic acids represent an important strategy for specific and facile detection of a target molecule in a complex solution, with many applications in chemistry, biology, medicine, and biotechnology. A biosensor requires a recognition module, a signal output module, and coupling between the two. Most protein-based biosensors designed to date utilize natural protein as the recognition module. The limited repertoire of natural binding proteins is an impediment to the generation of biosensors for a broader range of target molecules. Hellinga *et al.* designed new ligand binding functions into a protein involved in sugar sensing, demonstrating the possibility of significantly expanding the variety of biosensors (1). However, their system based on bacterial sugar-binding proteins appears to be limited to recognizing small molecules. Bacterial periplasmic peptide-binding proteins serve as sensors for peptide-based signaling (2). They may be a promising platform for developing peptide sensors, but to date no such sensors have been reported (3, 4).

Recent advances have enabled one to produce recombinant antibody fragments such as the Fab and single-chain Fv for diverse types of antigens (5). Similarly, binding proteins based on nonantibody scaffolds show considerable promise as alternatives to antibodies (6). Although these engineered binding proteins can serve

as recognition modules, there is no general strategy for converting them into sensors. The antibody and other commonly used scaffolds are highly rigid and consequently do not undergo large conformational changes upon target binding. These characteristics make them ill suited as platforms for sensor design through conformational coupling and consequently necessitate laborious development (7, 8). Antibody-based sandwich ELISA (enzyme-linked immunosorbent assay) is widely used for detecting and quantifying a target molecule but requires a pair of antibodies that can simultaneously bind to a given target, a requirement that is difficult to meet particularly for a small target (9).

Short peptide motifs containing a chemical signature (*e.g.*, the free C-terminus and phosphorylation) are important biomarkers involved in signal transduction and protein assemblies (10, 11). Such motifs are often recognized by the so-called modular interaction domains, and strategies have been developed to convert modular interaction domains into biosensors by coupling binding and folding (12, 13). While these strategies can be generalized, the repertoire of natural peptide-binding domains is limited, and they usually have low levels of affinity and specificity, limiting the utility of biosensors constructed in this manner. Furthermore, these design strategies require a sensor to be marginally stable so that its folding can be triggered by ligand binding, which

**ABSTRACT** Optical biosensors for short peptide motifs, an important class of biomarkers, have been developed based on “affinity clamps”, a new class of recombinant affinity reagents. Affinity clamps are engineered by linking a peptide-binding domain and an antibody mimic domain based on the fibronectin type III scaffold, followed by optimization of the interface between the two. This two-domain architecture allows for the design of allosteric coupling of peptide binding to fluorescence energy transfer between two fluorescent proteins attached to the affinity clamp. Coupled with high affinity and specificity of the underlying affinity clamps and rationally designed mutants with different sensitivity, peptide concentrations in crude cell lysate were determined with a low nanomolar detection limit and over 3 orders of magnitude. Because diverse affinity clamps can be engineered, our strategy provides a general platform to generate a repertoire of genetically encoded, label-free sensors for peptide motifs.


\*Corresponding author,  
skoide@uchicago.edu.

Received for review November 10, 2009  
and accepted January 29, 2010.

Published online February 9, 2010

10.1021/cb900284c

© 2010 American Chemical Society

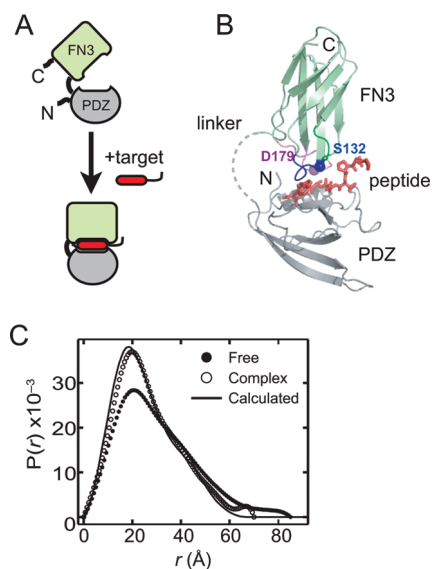

**Figure 1. Architecture and ligand-induced conformational change of an affinity clamp.** A) Schematic drawing of an affinity clamp. PDZ corresponds to the capture domain and FN3 to the enhancer domain. The ePDZ affinity clamps were developed by optimizing the binding interface of the FN3 domain through phage-display library selection. Ligand-induced conformational change of the affinity clamp is also indicated. B) The crystal structure of the ePDZ-a affinity clamp in complex with the ARVCF peptide (16). The PDZ domain, FN3 domain, and the peptide are shown in gray, pale green, and red, respectively. The linker connecting the PDZ and FN3 domains was disordered. Sites of mutations used in this work are also indicated. C) The  $P(r)$  curves derived from SAXS data for free ePDZ-a and of the ePDZ-a/peptide complex. A  $P(r)$  curve is the Fourier transformation of the SAXS data and indicates the distribution of mass-weighted atom–atom distances. The line shows a prediction from the crystal structure of the ePDZ-a/peptide complex.

reduces its sensitivity and *in vivo* stability. Also, although it is possible to envision adopting existing sensor technologies such as nucleotide aptamers, molecular beacons, and bacterial sensor proteins (1, 14, 15), it is not clear whether high levels of binding specificity for peptide motifs can be engineered into these systems. Together there

are urgent needs for a technology to generate highly specific and sensitive sensors for peptide motifs.


Here we report an integrated approach to generate high-performance affinity reagents for short peptide motifs and then convert them into label-free optical biosensors. Our strategy is based on a new type of binding proteins termed “affinity clamps” that have high affinity and high specificity to a short peptide motif (16). We found that target binding induces a large conformational change of an affinity clamp, which was exploited to construct genetically encoded, ratiometric sensors.

**Ligand-Induced Conformational Change of Affinity Clamps.** We have recently established a new protein-engineering strategy termed “directed domain-interface evolution” to generate affinity reagents to short peptide motifs with high affinity and exquisite specificity (16, 17). This strategy first genetically attaches an inert protein scaffold (“enhancer” domain) to a natural peptide-binding domain (“capture” domain). Subsequently, a combinatorial phage-display library is constructed in which portions of the enhancer domain are diversified. High-affinity variants with an optimized enhancer domain are then selected. Using the fibronectin type III (FN3) domain as the enhancer, we have dramatically enhanced the binding affinity and specificity of the erbin PDZ domain (18), an interaction domain with weak affinity to the C-terminal extreme of target proteins (Figure 1, panels A and B). We have termed these two-domain proteins affinity clamps. The architecture of affinity clamps is distinctly different from those of common affinity reagents (*e.g.*, antibodies) in that the target recognition site is constructed at the interface between two domains that are loosely connected with a short linker. Consequently, target binding may induce a large change in the relative orientation of the two domains (Figure 1, panel A), which could be allosterically coupled to a read-out mechanism for a biosensor.

Small-angle X-ray scattering (SAXS) analysis of an affinity clamp, termed ePDZ-a, revealed large conformational change induced by ligand binding. This affinity clamp binds to the C-terminal peptide motif, PQPVDSWV-COOH, derived from a human protein, ARVCF (Armadillo repeat gene deleted in Velo-cardio-facial syndrome) (16, 18). Upon an addition of a 10-residue peptide that contains the binding motif GG-PQPVDSWV, we observed a significant change in the SAXS profile (Figure 1, panel C), suggesting a large change in interdomain orientation of the affinity clamp.

**Sensor Design.** To couple the observed conformational change with optical read out, the affinity clamp was genetically fused to a pair of FRET-optimized fluorescent proteins (FPs), CyPet and YPet (19), with CyPet at the N-terminus of ePDZ-a and YPet at the C-terminus (Figure 2, panel A). This FP pair exhibits a large FRET change upon dissociation, because surface mutations in them increase their tendency to heterodimerize when they are linked within a single polypeptide and achieve a high FRET efficiency (20–22). A similar set of “sticky” FPs has been used to develop a zinc sensor, eCALWY-1, in which zinc binding to a zinc-recognition module disrupts heterodimerization of the FP pair (23). We envisioned that the conformational change of the affinity clamp could be similarly exploited to develop FRET sensors.


The resulting fusion protein CyPet-ePDZ-a-YPet was produced in *E. coli*. In the absence of an added peptide, the fluorescence emission spectrum of the fusion protein with excitation of CyPet at 415 nm exhibited an intense peak at 527 nm (Figure 2, panel B), similar to the spectrum of CyPet and YPet linked with a short peptide (19). As the target peptide was added, the spectrum of the fusion protein showed large changes. The overall decrease in the intensity of the YPet emission peak at 527 nm was ~50% corresponding to a FRET ratio change of ~250% (Figure 2, panel B), a

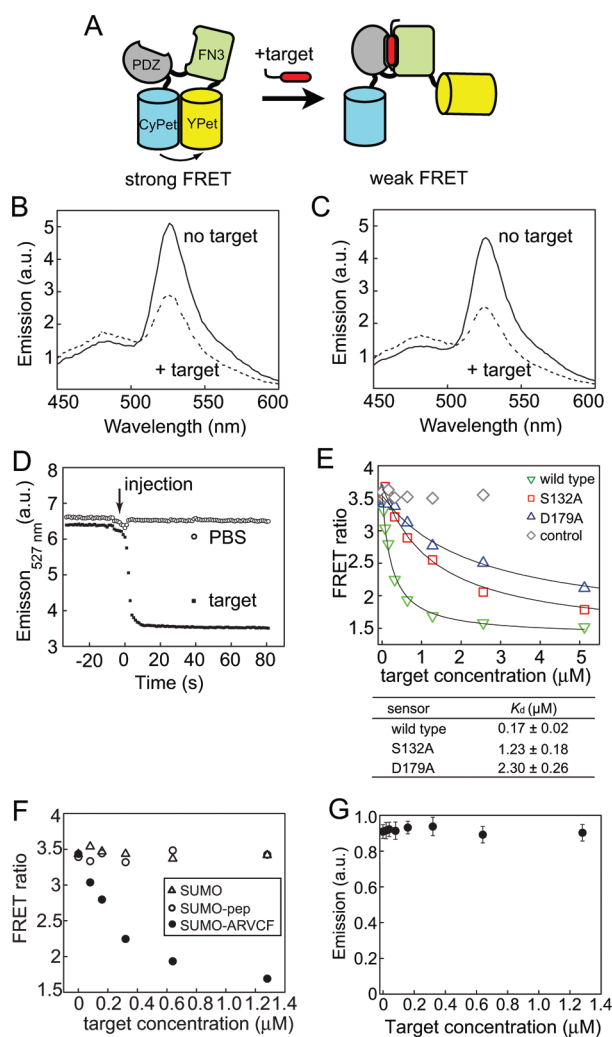

**Figure 2.** Clamp sensor design and characterization. **A)** Schematic drawing of the design principle. The closure of the affinity clamp alters interactions between the two fluorescent proteins, CyPet and YPet, affecting the FRET efficiency. **B)** Fluorescence emission spectra of the clamp sensor in PBS in the presence and absence of the target peptide ( $1.2 \mu\text{M}$ ) with excitation at 415 nm. **C)** Fluorescence emission spectra of the clamp sensor in the presence and absence of the SUMO-ARVCF fusion protein ( $1.2 \mu\text{M}$ ). **D)** Response time course of the clamp sensor. Fluorescence emission intensity at 527 nm with excitation at 415 nm is plotted as a function of time, as a saturating concentration of peptide was injected. The intensity was monitored every second. **E)** FRET ratios (emission at 527 nm over emission at 475 nm) of clamp sensors in PBS plotted as a function of SUMO-ARVCF concentration. Responses of three different sensors are shown. “Control” is a nonfunctional sensor containing an FN3 domain that does not bind to the target. The data points at 10 and 20  $\mu\text{M}$  are omitted for clarity. The curves show the best fit of a 1:1 binding model. The  $K_d$  values are also shown. **F)** Responses of the wild-type clamp sensor to SUMO-ARVCF, SUMO with no attached peptide, and a SUMO fusion with an unrelated peptide (“SUMO-pep”; GGDVHVNATYVNVKSVA). The FRET ratios are plotted as a function of ligand concentration. **G)** Fluorescence emission intensity at 527 nm of YPet with excitation at 514 nm plotted as a function of SUMO-ARVCF concentration, showing that the quantum yield of YPet is not affected by peptide binding.

magnitude similar to those observed for other FP-based biosensors (23–25). Similar results were observed when the target peptide was attached to a small protein, yeast SUMO via a short linker (referred to as SUMO-ARVCF hereafter; Figure 2, panel C), indicating that the sensor can recognize the ARVCF peptide motif attached to a protein equally well. Because of the ease of production and quantification of SUMO-ARVCF fusion protein, we used SUMO-ARVCF as a target for subsequent experiments. The sensor showed rapid response to a change in peptide concentration with an apparent relaxation time of a few seconds (Figure 2, panel D). The titration data (Figure 2, panel E) gave a  $K_d$  value of  $170 \pm 20 \text{ nM}$ ,  $\sim 3$ -fold larger than the  $K_d$  of isolated ePDZ-a ( $56 \pm 5 \text{ nM}$ ). As expected, a control construct, with an FN3 domain with no appreciable binding to the target peptide, did not change the emission upon target addition (Figure 2, panel E). Similarly, SUMO without an attached peptide or SUMO fused with an unrelated peptide had no significant effect on the FRET ratio of the wild-type sensor (Figure 2, panel F). These results validate our strategy in converting an affinity reagent into a biosensor. We name this class of biosensors clamp sensors.

Several lines of evidence support a model for the mechanism of the clamp sensor (Figure 2, panel A) in which conformational changes of the affinity clamp disrupt optimal dimerization of CyPet and YPet necessary for efficient FRET. Our sensor exhibited a decrease, rather than increase, in YPet emission upon peptide binding. Peptide addition did not affect the YPet emission when YPet was directly excited (Figure 2, panel G), indicating that the peptide binding to the affinity clamp did not affect the quantum yield of YPet. The  $K_d$  of the clamp sensor was increased relative to that of the underlying affinity clamp, similar to a 10-fold  $K_d$  increase observed for the eCALWY-1 zinc sensor designed using the same principle (23). Together, these results strongly sup-

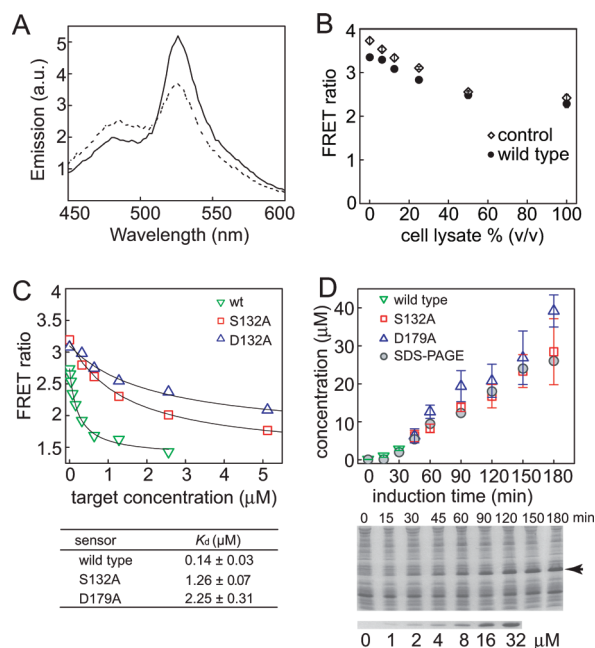

**Figure 3. Peptide quantification in cell lysate using clamp sensors.** **A)** Fluorescence emission spectra of the clamp sensor in crude cell lysate in the presence and absence of SUMO-ARVCF (2 μM). **B)** Effects of cell lysate on the FRET ratio of the clamp sensor. The FRET ratios of the wild-type sensor and a negative control sensor (as described in Figure 2, panel E) are plotted versus the concentration of cell lysate. Measurements were taken in the absence of a target peptide. **C)** FRET signals of clamp sensors in cell lysate plotted as a function of SUMO-ARVCF concentrations. **D)** Measurements of SUMO-ARVCF expression in *E. coli* cell lysates with the clamp sensors. The concentrations of SUMO-ARVCF at different time points after the initiation of expression were determined. The protein levels were also estimated from SDS-PAGE (middle panel; the arrow indicates the band for SUMO-ARVCF) of cell lysates using SUMO-ARVCF of known concentrations as standards (lower panel).

port that the observed changes in YPet emission are due to changes in FRET efficiency between CyPet and YPet. The relatively small changes in the CyPet emission at 475 nm appear to be characteristic of sensors constructed with the CyPet-YPet pair, as observed previously (19). It is notable that a large level of emission change was achieved without optimizing the linkers between the affinity clamp and the fluorescent proteins, consistent with a view that disruption of a sticky FP pair may be an effi-

cient strategy for developing FRET sensors (22, 23).  
**Rational Modulation of Clamp Sensor Sensitivity.** A series of sensors with different sensitivity would expand the detection range and thus can increase their utility. On the basis of the crystal structure of ePDZ-a in complex with the ARVCF peptide (16), we identified S132 and D179 located in the loops of FN3 that form the peptide-binding interface as potential sites for mutation (Figure 1, panel B). S132 forms a hydrogen bond with the target peptide. D179 forms multiple hydrogen bonds with other FN3 residues, which appeared to stabilize the loop conformation for binding. The S132A and D179A mutants of the clamp sensor showed, respectively, 7.2- and 13.5-fold reduced affinity relative to that of the wild-type sensor (Figure 2, panel E). Importantly, they maintained the sensor characteristics in terms of the FRET ratios in the absence

of the target and the total change upon saturation estimated from curve fitting (Figure 2, panel E). Thus, we have successfully altered the sensitivity of the clamp sensor without diminishing its signal transduction property.  
**Applications of the Clamp Sensors.** The utility of these clamp sensors was further illustrated by determining the concentration of the target peptide motif in crude cell lysate. The responses of the clamp sensor in cell lysate were similar to those observed in

PBS, indicating that the clamp sensor was not significantly influenced by other molecules in cell lysate, as expected from exquisite specificity of the affinity clamp used (Figure 3, panels A and C). These results further support high specificity of the affinity clamp used. We noted that the absolute values for the FRET ratio were different in cell lysate from those in PBS (Figure 2, panel E). This difference was caused by the cell lysate altering the FRET profile between YPet and CyPet, probably by affecting their association (Figure 3, panel B). However, this effect can easily be accounted for by establishing a calibration curve in the presence of cell lysate. Then, we used the clamp sensors to determine the concentration of SUMO-ARVCF expressed in *E. coli* at different time points after induction of protein expression. The protein concentrations determined with the clamp sensors agreed well with those estimated from SDS-PAGE (Figure 3, panel D). These results demonstrate that the clamp sensor provides a robust and highly sensitive method to measure the absolute protein concentrations in a complex mixture.

In conclusion, we have described a rational strategy to convert affinity clamps into label-free, ratiometric fluorescence sensors for peptide biomarkers. Affinity clamps with different binding properties can be generated by replacing and/or mutating the capture domain and the overall architecture of affinity clamps is conserved regardless of their target. Therefore, we speculate that we can establish an integrated pipeline to simultaneously generate high-quality affinity reagents and label-free biosensors for diverse peptide motifs, which would make large impacts on cell biology, biotechnology, and medicine. Furthermore, because clamp sensors can be genetically encoded and expressed in the functional form in cells, we speculate that they could be used to monitor real-time changes in biomarker concentration and localization in living cells.

## METHODS

**Protein Expression and Purification.** The ePDZ-a and SUMO-ARVCF proteins were prepared as described previously (16). The amino acid sequence for SUMO-ARVCF is mkhhhhhhssdykdddkge-nlyfqg-SDSEVNQEAQPEVKPEVKPETHINLKVSD-GSSEIFFKIKKTTPLRRLMEAFKRQKEMDSLRFYDGIQADQTPEDLDMEDNDIIEAHQIGGGPQPVDVSWY, where the segment in lower case encodes His<sub>6</sub> and FLAG tags, and the ARVCF peptide is underlined. Its molecular weight is 15.3 kDa. BL21(DE3) cell lysates were prepared by treating cell suspension with 0.5 mg mL<sup>-1</sup> lysozyme containing 1 mM PMSF in 50 mM Tris-HCl buffer (pH 8) followed by sonication. Lysates were cleared with centrifugation and protein concentration was estimated with SDS-PAGE using Phast-System (Amersham) and CBB staining. The lysates were diluted 10–15× in PBS prior to fluorescence measurement.

**Small Angle X-ray Scattering.** Data were collected at the BioCAT beamline at the Advanced Photon Source, Argonne National Laboratory. Samples were prepared at a final protein concentration of 1 mg mL<sup>-1</sup> in TBS pH 7.5. For complex formation, the peptide was added at 1.2:1 ratio to the protein. Buffer blanks and samples were flowed through a 1.5 mm capillary at a rate of 2 μL s<sup>-1</sup> and 15 exposures of ~1 s duration were collected. The exposures were averaged, buffer blanks subtracted, and Guinier analysis performed using IGOR Pro (Wave Metrics). I(Q) data were converted to P(r) data using GNOM (26). P(r) data were normalized to an area proportional to (molecular weight)<sup>2</sup>.

**Clamp Sensor Construction and Purification.** The vectors for CyPet and YPet were made available by Dr. P. Daugherty through Addgene (19). The CyPet gene was cloned between the NheI and BamHI sites of pET24a (Novagen), and the Ypet gene was cloned between the EcoRI and XhoI sites of the resulting plasmid to yield a plasmid, pCypetYpet. The ePDZ-a gene was then inserted between the BamHI and XhoI sites of pCypetYpet. There was no linker between CyPet and ePDZ-a, and a four-residue linker (GGLE) was used between ePDZ-a and YPet. The CyPet-ePDZ-a-YPet fusion gene was expressed in BL21(DE3) cells and purified using Ni affinity chromatography. Mutant sensors were constructed using Kunkel mutagenesis (27).

**Fluorescence Measurements.** The clamp sensor was used at 140 nM unless otherwise noted. For titration, samples were placed in a black flat-bottom 96-well plate (Corning COSTAR), degassed, and incubated at 25 °C for 30 min in the dark prior to measurement in using a Tecan Safire (2) plate reader. An excitation wavelength of 415 nm was used unless otherwise stated. The K<sub>d</sub> was determined by fitting a 1:1 binding model to the emission ratio (emission at 527 nm/emission at 475 nm) as a function of peptide concentration:

$$F = F_0 + \Delta F$$

$$\left( \frac{[S_0] + [L_0] + K_d - \sqrt{([S_0] + [L_0] + K_d)^2 - 4[S_0][L_0]}}{2[S_0]} \right)$$

where  $F$  is the observed fluorescence intensity,  $F_0$

is the fluorescence intensity in the absence of a target peptide,  $\Delta F$  is the change in fluorescence upon sensor saturation,  $S_0$  is the total sensor concentration, and  $L_0$  is the total target concentration.

To determine the SUMO-ARVCF concentration in crude lysates, a sensor calibration curve was made using cell lysates containing known concentrations of SUMO-ARVCF. The intensities of protein bands in SDS-PAGE were analyzed using ImageJ (<http://rsbweb.nih.gov/ij/>).

The relaxation time of the clamp sensor was measured using a Aminco-Bowman AB-2 fluorometer with excitation at 415 nm and emission at 527 nm with 1 s interval. To a cuvette containing 0.23 μM sensor in PBS, SUMO-ARVCF was manually injected at a final concentration of 2 μM while the solution was vigorously mixed with a magnetic stirrer.

**Acknowledgment:** We thank T. Sosnick and D. Strickland for SAXS analysis and P. Daugherty for the CyPet and YPet genes. This work was supported by the National Institutes of Health grants R21-CA132700, R21-DA025725, and R01-GM090324 to S.K.

## REFERENCES

- Looger, L. L., Dwyer, M. A., Smith, J. J., and Hellinga, H. W. (2003) Computational design of receptor and sensor proteins with novel functions, *Nature* 423, 185–190.
- Perego, M. (1997) A peptide export-import control circuit modulating bacterial development regulates protein phosphatases of the phosphorelay, *Proc. Natl. Acad. Sci. U.S.A.* 94, 8612–8617.
- Tame, J. R., Murshudov, G. N., Dodson, E. J., Neil, T. K., Dodson, G. G., Higgins, C. F., and Wilkinson, A. J. (1994) The structural basis of sequence-independent peptide binding by OppA protein, *Science* 264, 1578–1581.
- Levdikov, V. M., Blagova, E. V., Brannigan, J. A., Wright, L., Vagin, A. A., and Wilkinson, A. J. (2005) The structure of the oligopeptide-binding protein, AppA, from *Bacillus subtilis* in complex with a nonapeptide, *J. Mol. Biol.* 345, 879–892.
- Bradbury, A. R., and Marks, J. D. (2004) Antibodies from phage antibody libraries, *J. Immunol. Methods* 290, 29–49.
- Binz, H. K., Amstutz, P., and Pluckthun, A. (2005) Engineering novel binding proteins from nonimmunoglobulin domains, *Nat. Biotechnol.* 23, 1257–1268.
- Hudson, P. J., and Souriau, C. (2003) Engineered antibodies, *Nat. Med.* 9, 129–134.
- Renard, M., Belkadi, L., Hugo, N., England, P., Altschuh, D., and Bedouelle, H. (2002) Knowledge-based design of reagentless fluorescent biosensors from recombinant antibodies, *J. Mol. Biol.* 318, 429–442.
- Hamaguchi, Y., Kato, K., Fukui, H., Shirakawa, I., and Okawa, S. (1976) Enzyme-linked sandwich immunoassay of macromolecular antigens using the rabbit antibody-coupled glass rod as a solid phase, *Eur. J. Biochem.* 71, 459–467.
- Pawson, T., and Nash, P. (2003) Assembly of cell regulatory systems through protein interaction domains, *Science* 300, 445–452.
- Bhattacharya, R. P., Remenyi, A., Yeh, B. J., and Lim, W. A. (2006) Domains, motifs, and scaffolds: the role of modular interactions in the evolution and wiring of cell signaling circuits, *Annu. Rev. Biochem.* 75, 655–680.
- Kohn, J. E., and Plaxco, K. W. (2005) Engineering a signal transduction mechanism for protein-based biosensors, *Proc. Natl. Acad. Sci. U.S.A.* 102, 10841–10845.
- Stratton, M. M., Mitrea, D. M., and Loh, S. N. (2008) A Ca<sup>2+</sup>-sensing molecular switch based on alternate frame protein folding, *ACS Chem. Biol.* 3, 723–732.
- Tyagi, S., and Kramer, F. R. (1996) Molecular beacons: probes that fluoresce upon hybridization, *Nat. Biotechnol.* 14, 303–308.
- Nutiu, R., and Li, Y. (2005) Aptamers with fluorescence-signaling properties, *Methods* 37, 16–25.
- Huang, J., Koide, A., Makabe, K., and Koide, S. (2008) Design of protein function leaps by directed domain interface evolution, *Proc. Natl. Acad. Sci. U.S.A.* 105, 6578–6583.
- Huang, J., Makabe, K., Biancalana, M., Koide, A., and Koide, S. (2009) Structural basis for exquisite specificity of affinity clamps, synthetic binding proteins generated through directed domain-interface evolution, *J. Mol. Biol.* 392, 1221–1231.
- Laura, R. P., Witt, A. S., Held, H. A., Gerstner, R., De-shayes, K., Koehler, M. F., Kosik, K. S., Sidhu, S. S., and Lasky, L. A. (2002) The Erbin PDZ domain binds with high affinity and specificity to the carboxyl termini of  $\delta$ -catenin and ARVCF, *J. Biol. Chem.* 277, 12906–12914.
- Nguyen, A. W., and Daugherty, P. S. (2005) Evolutionary optimization of fluorescent proteins for intracellular FRET, *Nat. Biotechnol.* 23, 355–360.
- Ohashi, T., Galiacy, S. D., Briscoe, G., and Erickson, H. P. (2007) An experimental study of GFP-based FRET, with application to intrinsically unstructured proteins, *Protein Sci.* 16, 1429–1438.
- Vinkenburg, J. L., Evers, T. H., Reulen, S. W., Meijer, E. W., and Merx, M. (2007) Enhanced sensitivity of FRET-based protease sensors by redesign of the GFP dimerization interface, *ChemBioChem* 8, 1119–1121.
- Campbell, R. E. (2009) Fluorescent-protein-based biosensors: modulation of energy transfer as a design principle, *Anal. Chem.* 81, 5972–5979.
- Vinkenburg, J. L., Nicolson, T. J., Bellomo, E. A., Koay, M. S., Rutter, G. A., and Merx, M. (2009) Genetically encoded FRET sensors to monitor intracellular Zn<sup>2+</sup> homeostasis, *Nat. Methods* 6, 737–740.
- Miyawaki, A., Llopis, J., Heim, R., McCaffery, J. M., Adams, J. A., Ikura, M., and Tsien, R. Y. (1997) Fluorescent indicators for Ca<sup>2+</sup> based on green fluorescent proteins and calmodulin, *Nature* 388, 882–887.
- Awais, M., Sato, M., Sasaki, K., and Umezawa, Y. (2004) A genetically encoded fluorescent indicator capable of discriminating estrogen agonists from antagonists in living cells, *Anal. Chem.* 76, 2181–2186.
- Semenyuk, A. V., and Svergun, D. I. (1991) GNOM—a program package for small-angle scattering data processing, *J. Appl. Crystallogr.* 24, 537–540.
- Kunkel, T. A., Roberts, J. D., and Zakour, R. A. (1987) Rapid and efficient site-directed mutagenesis without phenotypic selection, *Methods Enzymol.* 154, 367–382.