

# A New Cross-Linkable Oxygen Sensor Covalently Bonded into Poly(2-hydroxyethyl methacrylate)-*co*-Polyacrylamide Thin Film for Dissolved Oxygen Sensing

Yanqing Tian,\* Bradley R. Shumway, and Deirdre R. Meldrum

Center for Ecogenomics, Biodesign Institute, Arizona State University, 1001 McAllister Avenue, Tempe, Arizona 85287

Received November 3, 2009. Revised Manuscript Received January 15, 2010

A new oxygen sensor, compound **2**, was synthesized through a chemical modification of a popularly used oxygen sensor of platinum(II)-5,10,15,20-tetrakis-(2,3,4,5,6-pentafluorophenyl)-porphyrin (PtTFPP). The new sensor compound **2** possesses four cross-linkable methacrylate functional moieties, enabling it to be polymerized and cross-linked with other monomers for polymer sensing film (also called membrane) preparation. Using this characteristic, compound **2** was covalently bonded to hydrophilic poly(2-hydroxyethyl methacrylate)-*co*-polyacrylamide (referred to as PHEMA to simplify) and hydrophobic polystyrene (PS) films. To better understand the advantages and disadvantages of chemical cross-linking approaches and the influence of polymer matrices on sensing performance, we physically incorporated PtTFPP into the same PHEMA and PS matrices to compare. Response to dissolved oxygen (DO), leaching of the sensor molecules from their matrices, photostability of the sensors, and response time to DO changes were studied. It was concluded that the chemical cross-linking of the sensor compound **2** in polymer matrices: (i) alleviated the leaching problem of sensor molecules that usually occurred in the physically doped sensing systems, and (ii) significantly improved sensors' photostability. The PHEMA matrix was demonstrated to be more suitable for dissolved oxygen sensing than PS, because for the same sensor molecule, the oxygen sensitivity in PHEMA film was higher than that in PS and response time to DO change in the PHEMA film was faster than that in PS. It was the first time oxygen sensing films were successfully prepared using biocompatible hydrophilic PHEMA as a matrix, which does not allow leaching of the sensor molecules from the polymer matrix, has a faster response to DO changes than that of PS, and does not present cytotoxicity to human lung adenocarcinoma epithelial cells (A549). It is expected that the new sensor compound **2** and its similar compounds with chemical cross-linking characteristics can be widely applied to generate many interesting oxygen sensing materials for studying biological phenomena.

## 1. Introduction

Measurement of dissolved oxygen (DO) has attracted great attention because DO is highly related to water quality, food freshness, medication, scientific understanding of cell respiration and metabolism, and other physiological and biological applications.<sup>1</sup> Various types of oxygen sensors have been developed based on mechanisms such as pressure, electrochemistry, and fluorescence quenching (an optical approach).<sup>1</sup> Because sensors based on

emission quenching are noninvasive or minimally invasive, disposable, easily miniaturized (down to submicrometer), and simple to process (as a coating or solid layer on optical fibers or surfaces for remote measurement of chemical and biochemical parameters), the optical approach<sup>1b</sup> to DO measurement most interested us among the various mechanisms being used. We are using the optical oxygen sensors integrated with lab-on-a-chip devices for single cell metabolism studies.<sup>1j,k</sup>


Ruthenium(II) polypyridyl complexes,<sup>2</sup> platinum(II), and palladium(II) porphyrins,<sup>3</sup> and cyclometalated complexes

\*To whom all correspondence should be addressed. E-mail: yanqing.tian@asu.edu. Phone: (480) 965-9601. Fax: (480) 727-6588.

(1) (a) Amao, Y. *Mirochim. Acta.* **2003**, *143*, 1. (b) Nagl, S.; Wolfbeis, O. S. *Analyst* **2007**, *132*, 507. (c) Hitoshi, H.; Tsunee, I.; Toshiaki, M.; Kazahiro, K. *J. Oceanogr.* **2006**, *62*, 99. (d) Clark, L. C. *Trans. Am. Soc. Artif. Intern. Organs* **1956**, *2*, 41. (e) Evans, N. T. S.; Naylor, P. F. F. *Resp. Physiol.* **1967**, *3*, 38. (f) Huch, R.; Lubbers, D. W.; Huch, A. *Arch. Dis. Child.* **1974**, *49*, 213. (g) Köneke, R.; Comte, A.; Jürgens, H.; Kohls, O.; Lam, H.; Scheper, T. *Chem. Eng. Technol.* **1999**, *22*, 666. (h) Mitsubayashi, K.; Wakabayashi, Y.; Murotomi, D.; Yamada, T.; Kawase, T.; Iwagaki, S.; Karube, I. *Sens. Actuators, B* **2003**, *95*, 373. (i) Wang, X. D.; Chen, X.; Xie, Z.-X.; Wang, X. R. *Angew. Chem., Int. Ed.* **2008**, *47*, 7450. (j) Lidstrom, M. E.; Meldrum, D. R. *Nat. Rev. Microbiol.* **2003**, *1*, 158. (k) Molter, T. W.; McQuaide, S. C.; Suchorolski, M. T.; Strovas, T. J.; Burgess, L. W.; Meldrum, D. R.; Lidstrom, M. E. *Sens. Actuators, B* **2009**, *135*, 678.

(2) (a) García-Fresnadillo, D.; Marazuela, M. D.; Moreno-Bondi, M. C.; Orellana, G. *Langmuir* **1999**, *15*, 6451. (b) Amao, Y.; Okura, I. *Sens., Actuators B* **2003**, *88*, 162. (c) Xu, H.; Aylott, J. W.; Kopelman, R.; Miller, T. J.; Philbert, M. A. *Anal. Chem.* **2001**, *73*, 4124. (d) McEvoy, A. K.; McDonagh, C.; MacCraith, B. D. *J. Sol-Gel Sci. Technol.* **1997**, *8*, 1121. (e) Roche, P.; Al-Jowder, R.; Narayanaswamy, R.; Young, J.; Scully, P. *Anal. Bioanal. Chem.* **2006**, *386*, 1245. (3) (a) Borisov, S. M.; Vasylevska, A. S.; Krause, C.; Wolfbeis, O. S. *Adv. Funct. Mater.* **2006**, *16*, 1536. (b) Kimura, F.; Khalil, G.; Zettsu, N.; Xia, Y.; Callis, J.; Gouterman, N. M.; Dalton, L.; Dabiri, D.; Rodriguez, M. *Meas. Sci. Technol.* **2006**, *254*. (c) Köse, M. E.; Carrol, B. F.; Schanze, K. S. *Langmuir* **2005**, *21*, 9121. (d) McDonagh, C.; Burke, C. S.; MacCraith, B. D. *Chem. Rev.* **2008**, *108*, 400.

Scheme 1

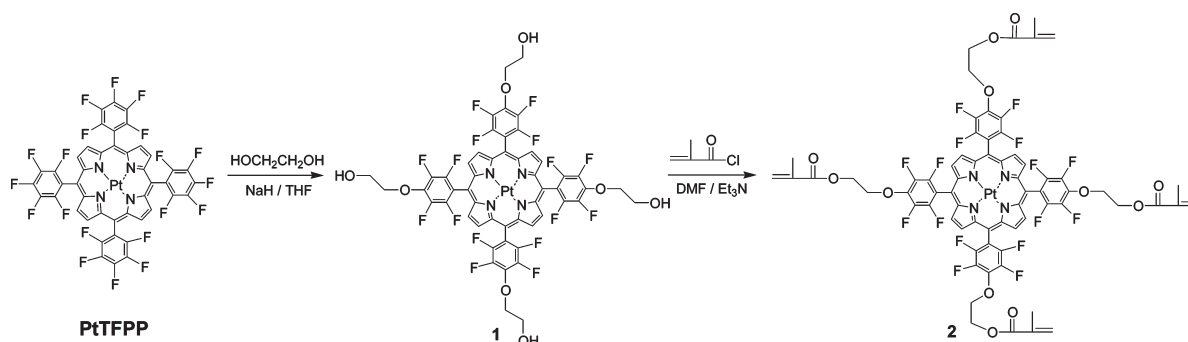

of platinum(II) and iridium(III)<sup>4</sup> are typical chemical materials acting as fluorescence-based oxygen sensors because of their long triplet state lifetime in the ranges of a few to tens of microseconds and sufficient triplet–triplet energy transfer from these compounds to oxygen molecules. This results in a decrease of the oxygen sensors' emission intensities and a shortening of their lifetimes by oxygen. Among the many oxygen sensors, platinum(II)-5,10,15,20-tetrakis-(2,3,4,5,6-pentafluorophenyl)-porphyrin (PtTFPP) is believed to be an excellent sensor because of its good response to oxygen concentrations and high photostability as compared with others.<sup>5</sup> To realize the measurement of DO in liquids, we usually physically incorporated oxygen sensing molecules and dispersed them in various hydrophobic matrices with good oxygen permeability<sup>2–4</sup> including silicon rubbers, silica gels, organosilicas, polystyrene, cellulose derivatives, and polyurethane-type hydrogels.

Biocompatible polymers, such as collagen, poly(2-hydroxyethyl methacrylate) (PHEMA), and poly[*N*-(2-hydroxypropyl) methacrylamide] (PHPMA) have been well-applied as hydrogels and scaffolds to study cell growth, proliferation, differentiation, and in studying cell function in 3D environments.<sup>6</sup> However, there is almost no report about using these biocompatible hydrogels as matrices for optical sensing studies because of the concern of significant leaching of the physically dispersed sensor molecules from these hydrophilic matrices. The leaching is undesired for applications for DO measurements because it may result in problems of signal instability, inaccuracy of measurements, decreased long-term applicability, and toxicity for cells. Successful preparation of optical oxygen sensors using the biocompatible gels as matrices with good oxygen sensitivity, photostability, reasonable response time, noncytotoxicity, and nonleaching of the sensors from their matrices is highly expected for bioapplications.


Herein, we developed a new oxygen sensor **2** shown in Scheme 1, which is a modified PtTFPP possessing four methacrylate moieties which can be easily mixed with hydrogel precursors (e.g., a mixture of 2-hydroxyethyl methacrylate (HEMA) and acrylamide) in a solvent (e.g., *N,N'*-dimethylformamide (DMF)) and polymerized/cross-linked to generate polymer hydrogels (e.g., PHEMA hydrogel) with chemically bonded sensors. Using about 20 wt% acrylamide as a comonomer with HEMA is for improving the matrix's ion permeability for a further integration of the sensing film with other sensors such as pH, K<sup>+</sup>, Ca<sup>2+</sup>, and Na<sup>+</sup> ion sensors for simultaneous measurement of multiparameters. The polymers can be prepared with controlled thickness as thin films or membranes. For a demonstration of excellent characteristics of the covalently bonded sensors in the PHEMA films, we also (1) chemically immobilized sensor monomer **2** to the popularly used hydrophobic polystyrene (PS) matrix to study the influence of matrices on sensing performance and (2) physically dispersed PtTFPP, the precursor for compound **2**, in the PS and PHEMA matrices to compare the covalently bonded and physically incorporated sensors on sensors' photostability and leaching. Interferences by ions, pH values, media, and temperatures on the PHEMA sensing films with covalently linked sensor compound **2** were studied. Toxicity of the new sensor film with covalently bonded sensor molecules to human lung cancer A549 cells was also evaluated.

## 2. Results and Discussion

**Synthesis of the New Sensor 2.** As outlined in Scheme 1, PtTFPP was first chemically modified using anhydrous ethylene glycol at a basic condition to generate compound **1**. The fluoride at para position of the meso-pentafluorophenyl group has a much higher chemical reactivity than other fluorides at the phenyl rings. This characteristic has been used to modify 5,10,15,20-tetrakis-(2,3,4,5,6-pentafluorophenyl)-porphyrin (TFPP) and platinum(II)-5,10,15,20-tetrakis-(2,3,4,5,6-pentafluorophenyl)-porphyrin (PtTFPP).<sup>7</sup>

- (4) (a) Vander Donckt, E.; Camerman, B.; Herne, R.; Vandeloise, R. *Sens. Actuators, B* **1996**, *32*, 121. (b) DeRosa, M.; Mosher, P.; Yap, G.; Foscanneau, K.; Crutchley, R.; Evans, C. *Inorg. Chem.* **2003**, *42*, 4864. (c) Borisov, S. M.; Klimant, I. *Anal. Chem.* **2007**, *79*, 7501. (d) Pauly, S. Permeability and Diffusion Data. In *Polymer Handbook*, 3rd ed.; Brandrup, J.; Immergut, E. H., Eds.; John Wiley & Sons: New York, 1989; Chapter 6, pp 435–449.
- (5) (a) Lee, S. K.; Okura, I. *Anal. Commun.* **1997**, *34*, 185. (b) Han, B. H.; Manners, I.; Winnik, M. A. *Anal. Chem.* **2005**, *77*, 8075.
- (6) (a) Hejcl, A.; Lesny, P.; Pradny, M.; Michalek, J.; Jendelova, P.; Stulik, J.; Sykova, E. *Physiol. Res.* **2008**, *57*(Suppl. 3), S121. (b) Bryanta, S. J.; Cuy, J. L.; Hauch, K.; Ratner, B. D. *Biomaterials* **2007**, *28*, 2978. (c) Schneider, G. B.; English, A.; Abraham, M.; Zaharias, R.; Stanford, C.; Keller, J. *Biomaterials* **2004**, *25*, 3023.

- (7) (a) Chen, X.; Hui, L.; Foster, D. A.; Drain, C. M. *Biochemistry* **2004**, *43*, 10918. (b) Samaroo, D.; Soll, C. E.; Todaro, L. J.; Drain, C. M. *Org. Lett.* **2006**, *8*, 4985. (c) Králóvá, J.; Bríza, T.; Moserová, I.; Dolenský, B.; Vašek, P.; Poučková, P.; Kejík, Z.; Kaplánek, R.; Martásek, P.; Dvořák, M.; Král, V. *J. Med. Chem.* **2008**, *51*, 5964. (d) Hirohara, S.; Obata, M.; Alitomo, H.; Sharyo, K.; Ando, T.; Yano, S.; Tanihara, M. *Bioconjugate Chem.* **2009**, *20*, 944.

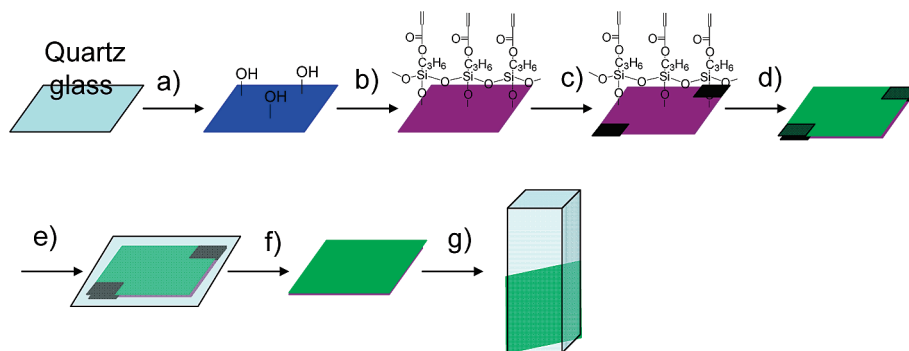

**Figure 1.** Schematic illustration of the preparation of sensing membranes: (a) oxygen plasma treatment to generate active hydroxyl groups; (b) vapor deposition of thin TMPSA layer; (c) 25  $\mu\text{m}$  tape used to control membrane thickness; (d) sensor solution dispensed onto modified quartz surface; (e) solution covered with a cover glass and polymerized at 80  $^{\circ}\text{C}$  for 1.5 h; (f) cover glass and tape removed; film rinsed using methanol and double-distilled water; and (g) sensing membrane on quartz substrate immersed into liquid in cuvette for fluorescence measurements.

**Table 1. Responses of the Sensing Films to Dissolved Oxygen in pH 7.0 B-R Buffer**

samples	sensor	matrix	conc. <sup>b</sup>	$\lambda_{\text{ex}}$ <sup>c</sup>	$\lambda_{\text{em}}$	$K_{\text{SV}}$ ( $\text{k Pa}^{-1}$ ) at various excitation wavelengths			
						394 nm	405 nm	508 nm	514 nm
F1	2	PHEMA <sup>a</sup>	0.1	394	649		0.0874 (0.9978) <sup>e</sup>		
F2	2	PHEMA <sup>a</sup>	1.0	394	649	0.0894; (0.9962)	0.0876; (0.9977)	0.0851; (0.9963)	0.0826; (0.9962)
F3	2	PHEMA <sup>a</sup>	10.0	389 <sup>d</sup>	649		0.073; (0.928)		
F4	PtTFPP	PHEMA <sup>a</sup>	1.0	394	650	0.1061; (0.9968)	0.1016; (0.9977)	0.1027; (0.9963)	0.0979; (0.9962)
F5	2	PS	0.1	395	650		0.0402; (0.9983)		
F6	2	PS	1.0	395	650	0.0392; (0.9987)	0.0380; (0.9987)	0.0377; (0.9984)	0.0374; (0.9982)
F7	2	PS	10.0	389 <sup>d</sup>	650		0.0378; (0.990)		
F8	PtTFPP	PS	1.0	394	650		0.045; (0.9979)		

<sup>a</sup> For simplification, the film of PHEMA and acrylamide copolymer was called PHEMA. <sup>b</sup> Conc: concentration in mg/g of sensor/matrix. <sup>c</sup>  $\lambda_{\text{ex}}$  in nm. Only the Soret band was listed in the table; the Q bands at 508 and 540 nm were not listed. <sup>d</sup> Broad peak. <sup>e</sup> Numbers in the parentheses are the correlation coefficients ( $R^2$ ) of the fitting.

After purification through column chromatography, **1** was then used to react with methacryloyl chloride to generate monomer **2** possessing four methacrylate moieties.

**Sensing Film (Membrane) Preparation.** A schematic procedure for the membrane preparation was given in Figure 1.


To achieve a stable polymer membrane on a substrate for optical characterization, a quartz substrate was modified with an acrylate-containing silane, trimethylsilylpropyl acrylate (TMPSA), using a vapor deposition approach.<sup>8</sup> The silane groups were anchored on the quartz surface with active hydroxyl groups generated by oxygen plasma treatments. The acrylate moiety can be further polymerized with other monomers to chemically graft the sensing membranes on the quartz surface. Contact angle of the quartz surface after the TMPSA modification was measured to be 60 $^{\circ}$ , whereas the contact angle of oxygen plasma-treated quartz before the vapor deposition was approximately 10 $^{\circ}$ . This difference indicated the successful surface modification of the quartz surface using TMPSA. To provide the polymer films with a good mechanical stability, ethyloxylate trimethylolpropane triacrylate (SR454) was used as a cross-linker. The membranes (films F1–F8, Table 1) were prepared through a solution polymerization of the monomers of **2**, **S** or HEMA/acrylamide, and SR454 in DMF via a variation of sensors, matrices and sensor concentrations. Thermal

polymerization initiated by azobisisobutyronitrile (AIBN) under nitrogen was used to cure the monomers for polymer immobilization on the quartz substrate. Thermal polymerization was used for polymer thin film generation not the popularly used photopolymerization approach in order to avoid the potential photobleaching problem for sensors<sup>9</sup> under short wavelength (usually 365 or 254 nm) photoexcitation. For a faster reaction, the polymerization was performed at 80  $^{\circ}\text{C}$ . It was found that under such conditions, uniform polymer membranes grafted on quartz surfaces were obtained after polymerization for 1.5 h under nitrogen. Typical pictures of a thin film with and without excitation by 365 nm were given in the Supporting Information (S-Figure 1). The film thickness distribution was also given in S-Figure 1. Increasing the polymerization time was not found to improve the film stability or vary the sensing performance. For our sensing studies, the thickness of the sensor membranes was controlled to approximately 25  $\mu\text{m}$ .


**Optical Properties of the Sensing Films.** Concentration-dependent excitation and emission spectra of sensor monomer **2** covalently bonded into poly(2-hydroxyethyl methacrylate)-co-polyacrylamide (referred to as PHEMA to simplify) (F1, F2, and F3 in Table 1) and PS (F5, F6, and F7 in Table 1) matrices were investigated in Britton-Robinson (B-R) pH 7.0 buffer. Typical spectra of F1, F2, and F3 were given in Figure 2. Three peaks at

(8) Hong, H. G.; Jiang, M.; Sligar, S. G.; Bohn, P. W. *Langmuir* **1994**, *10*, 153.

(9) Li, L.; Walt, D. R. *Anal. Chem.* **1995**, *67*, 3746.

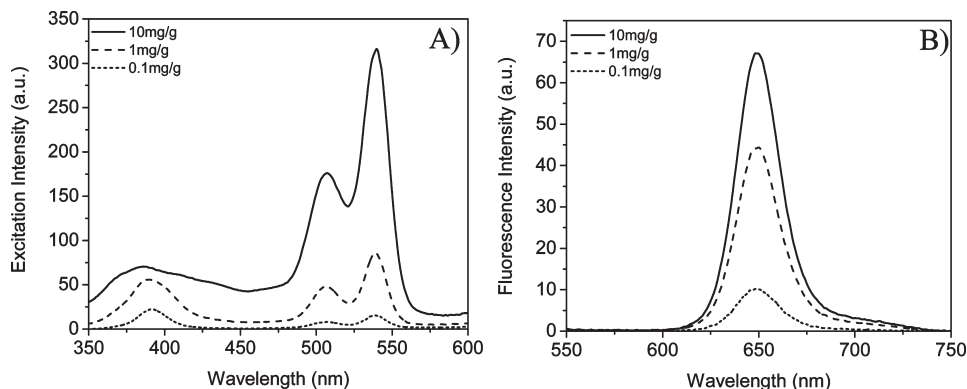

**Figure 2.** Concentration-dependent (A) excitation and (B) emission spectra of the sensors **2** covalently cross-linked on PHEMA matrix (films F1, F2, and F3). The units mg/g in the figures are weight ratios of the sensor in milligrams to polymer matrix in gram scale. For F1, 0.1 mg/g; F2, 1.0 mg/g; F3, 10.0 mg/g.

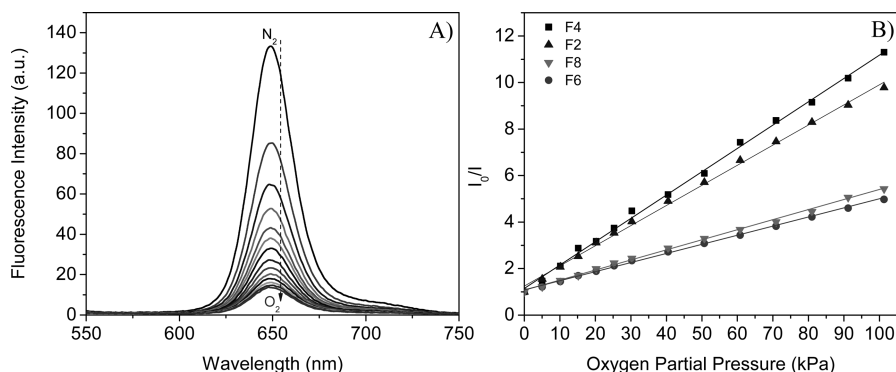

**Figure 3.** (A) Typical response to DO using F2 (covalently cross-linked **2** in PHEMA) in B-R pH 7.0 buffer and (B) the Stern–Volmer fittings for F2, F4 (physically doped PtTFPP in PHEMA), F6 (covalently cross-linked **2** in PS), and F8 (physically doped PtTFPP in PS) excited at 405 nm.  $I_0$  is the emission intensity in the deoxygenated buffer by flushing with nitrogen.  $I$  is the emission intensity of oxygen-containing solutions equilibrated with different oxygen partial pressures.

~390, 508, and 540 nm were observed in the excitation spectra corresponding to the Soret band and Q bands of platinum porphyrins.<sup>10</sup> Red emission was observed with a peak at 649 nm. The PtTFPP physically dispersed in the PHEMA hydrogel also exhibits similar photophysical properties (Table 1). Detailed studies about the structure influence on the photophysical properties of PtTFPP, compound **1** and compound **2** in solutions and films were given in Supporting Information, S-Figures 2 and 3. The fluorescence intensities did not have a linear dependence on the sensors' concentrations, showing a possibility of self-absorption<sup>11</sup> of the sensor molecules in the films. This may result in the self-quenching of the sensors, especially at higher concentration, such as 10 mg/g (sensor/gel), where the Soret-band around 390 nm became broad.

**Typical Oxygen Sensing (Film F2) for Dissolved Oxygen.** A mixture of oxygen and nitrogen gas was used to saturate aqueous solutions to tune dissolved oxygen concentrations by bubbling. Figure 3A shows typical DO response using chemically bonded **2** in PHEMA hydrogel F2. Fluorescence intensity of the oxygen sensor decreased with an increase in the dissolved oxygen concentration,

showing the good oxygen diffusion to the sensing membrane in aqueous solutions. Because the PHEMA hydrogel swells significantly in water,<sup>12</sup> the dissolved oxygen can interact efficiently with the sensor molecules to quench sensor's emissions. It has been well-known that the PHEMA hydrogel is an excellent material exhibiting good oxygen permeability for contact lenses.<sup>13</sup>

Intensity ratios ( $I_0/I$ ) of the F2 (Figure 3B) followed the Stern–Volmer equation with a correlation coefficient ( $R^2$ ) exceeding 0.997 as given in eq 1.

$$\frac{I_0}{I} = 1 + K_{SV}[\text{O}_2] \quad (1)$$

where  $K_{SV}$  is the Stern–Volmer quenching constant.  $I_0$  and  $I$  are the steady-state luminescence signals at 650 nm measured in deoxygenated and oxygen-containing solutions, respectively. Strictly speaking, the sensing membrane responds to DO ( $[\text{O}_2]$ ). However, because the actual oxygen concentration diffused into the polymer membrane was unknown, the partial pressure ( $p\text{O}_2$ ) of oxygen in the gas used to saturate the buffer was applied

(10) Rumyantseva, V. D.; Ivanovskaya, N. P.; Konovalenko, L. I.; Tsukanov, S. V.; Mironov, A. F.; Osin, N. S. *Russ. J. Bioorg. Chem.* **2008**, *34*, 239.  
 (11) Xiang, H.-F.; Yu, S.-C.; Che, C.-M.; Lai, P. T. *Appl. Phys. Lett.* **2003**, *83*, 1518.

(12) (a) Montheard, J.-P.; Chatzopoulos, M.; Chappard, D. *Polym. Rev.* **1992**, *32*, 1. (b) Parker, J. W.; Cox, M. E. *J. Polym. Sci. A: Polym. Chem.* **1988**, *26*, 1179.  
 (13) (a) Fornasiero, F.; Krull, F.; Prausnitz, J. M.; Radke, C. J. *Biomaterials* **2005**, *26*, 5704. (b) Wang, Y.; Tan, G.; Zhang, S.; Guang, Y. *Appl. Surf. Sci.* **2008**, *255*, 604.

in the above equation. The utilization of the oxygen partial pressure rather than the dissolved oxygen concentration in solutions has been widely accepted and used by other scientists,<sup>1b,9,14</sup> because the DO is proportional to the oxygen partial pressure. Standard atmosphere pressure of 101.3 kPa corresponds to an oxygen partial pressure of 21.3 kPa, and DO in air-saturated water at 20 °C under the standard pressure is 9.23 mg/L or 9.23 ppm.<sup>15</sup>

Excitation wavelengths had a slight effect on the Stern–Volmer quenching constants (Table 1). Besides the two wavelengths of the absorbance maxima at the Soret-band (394 nm) and the Q-band (508 nm), two widely applied laser excitation wavelengths (405 and 514 nm) in confocal fluorescence microscopy were chosen for comparison. Only slightly smaller quenching constants were observed when the excitation wavelengths were longer.

Concentration dependent Stern–Volmer quenching constants were also given in Table 1. It was found that the  $K_{SV}$  had some differences at different concentrations. Especially at a high concentration of 10 mg/g (sensor/gel), the quenching constant was much smaller, probably because of the self-aggregations of the sensor molecules in the membranes. On the basis of these results, the ratio of sensors to matrices of 1 mg/g for sensing performance investigation was usually chosen in order to achieve a good signal-to-noise ratio.

**Effects of Chemically Bonded Approach, Physically Doped Method, and the Matrices on Oxygen Sensing.** All of the sensor films from F1 to F8 (Table 1) showed linear Stern–Volmer responses to DO. However, sensitivity to DO was related to the film preparation approaches and matrices. The influence was reflected in the  $K_{SV}$  quenching constants. A larger  $K_{SV}$  indicated a higher sensitivity to DO. Typical plots using films F2 (chemically cross-linked **2** in PHEMA), F4 (physically incorporated PtTFPP in PHEMA), F6 (chemically bonded **2** in PS), and F8 (physically doped PtTFPP in PS) with the same sensor concentration (1 mg sensor in 1 g matrix) and the same excitation wavelength (405 nm) were given in Figure 3B, and more detailed data were given in Table 1.

Under a same condition,  $K_{SV}$  of F4 is larger than F2. Similarly,  $K_{SV}$  of F8 is larger than F6. These results showed that the chemical cross-linking of the sensor molecules **2** in the PHEMA and PS matrices made the films less sensitive to oxygen than the sensor molecules PtTFPP dispersed physically in the same matrices. The chemical cross-linking of the sensor molecules in the matrices probably restricted the molecule movements inside the matrix and slightly prohibited the interactions with oxygen molecules, resulting in a smaller quenching constant.

For the same sensor using the same film preparation method, the  $K_{SV}$  in PHEMA is almost twice of the  $K_{SV}$  in

PS (F2 vs F6 or F4 vs F8), showing a significant influence of the polymer matrices on the oxygen sensing and suggesting the PHEMA hydrogel is a better matrix for DO sensing than the hydrophobic PS. One reason is that the oxygen diffusion coefficient of PS ( $1.1 \times 10^{-8}$  to  $2.3 \times 10^{-7}$  cm<sup>2</sup>/s)<sup>16</sup> is much smaller than that of the swollen PHEMA ( $8 \times 10^{-7}$  to  $2.2 \times 10^{-6}$  cm<sup>2</sup>/s)<sup>12</sup> in aqueous solutions.


**Leaching Study of the Sensing Membranes.** The membranes with chemically bonded and physically trapped sensors were immersed in pH 7 B-R buffer and methanol, respectively, at room temperature to study the leaching of sensor molecules from polymer matrices. If the sensor molecules leach out of the sensing membranes and disperse in the polar solvents such as water and methanol, the total emission intensity of the sensing membranes and media will decrease as the emission of the oxygen sensor molecules will be quenched significantly by polar solvents. Significant emission decays, 15% for F4 in B-R buffer over 48 h, and 67% for F8 in methanol over only 16 h, were observed. Meanwhile, relatively weak PtTFPP emission was observed in B-R buffer and methanol, indicating that PtTFPP molecules leached out from their matrices. These results clearly showed the instability of sensing films made through the physical trapping approach when used for dissolved oxygen study, whereas sensing films with covalently bonded sensors alleviated the leaching problem. For the sensor films F2 and F6, there was no observed emission intensity difference before and after 48 h of soaking in buffer or methanol.

**Response Time Studies Using F2 and F6.** Figure 4 shows the response time and operational stability of the sensing films F2 (**2** cross-linked in PHEMA) and F6 (**2** cross-linked in PS) in pH 7.0 B-R buffer, which was conducted by measuring the intensity signal during alternated saturation of the solution with oxygen and nitrogen.


For F2, the response times,  $t_{95}$  (i.e., the time for 95% of the total change in fluorescence intensity to occur) and  $t_{99}$  (i.e., the time for 99% of the total change in fluorescence intensity to occur), were 50 and 70 s from the deoxygenated buffer to 100% oxygenated solution (Figure 4A), respectively. Recovery times from the oxygenated solution to deoxygenated solution were slower with a  $t_{95}$  of 240 s and  $t_{99}$  of 285 s. For F6, the response time  $t_{95}$  was 84 s and  $t_{99}$  was 182 s. The recovery times were much slower with a  $t_{95}$  of 420 s and  $t_{99}$  of 540 s (Figure 4B). Slow response times of sensors in PS for DO were previously reported in the range of 2–5 min,<sup>2d,17a</sup> although the same sensors can respond much more rapidly to oxygen gas in the range of 2 to 5 s. Some silica gel sensing films were reported to have slow DO response time of about 2 min.<sup>2e,17b</sup> Another type of sensing film using Nafilon<sup>2a,17c</sup> as the matrix was also reported to have a response time of

(14) (a) Wolfbeis, O. S. *J. Mater. Chem.* **2005**, *15*, 2657. (b) Vasylevska, G. S.; Borisov, S. M.; Krause, C.; Wolfbeis, O. S. *Chem. Mater.* **2006**, *18*, 4609. (c) Schröder, C. R.; Polerecky, L.; Klimant, I. *Anal. Chem.* **2007**, *79*, 60. (d) Kocincova, A. S.; Arain, S. N.; Krause, C.; Borisov, S. M.; Arnold, M.; Wolfbeis, O. S. *Biotechnol. Bioeng.* **2008**, *100*, 430. (15) Rooney, P. C.; Daniels, D. D. *Pet. Technol. Q.* **1998**, *Q2*, 97.

(16) (a) Kneas, K. A.; Demas, J. N.; Nguyen, B.; Lockhart, A.; Xu, W.; DeGraff, B. A. *Anal. Chem.* **2002**, *74*, 1111. (b) Gao, Y.; Ogilby, P. R. *Macromolecules* **1992**, *25*, 4962. (17) (a) Trettnak, W.; Gruber, W.; Reiningner, F.; O'Leary, P.; Klimant, I. *Adv. Space Res.* **1996**, *8*, 139. (b) McDonagh, C.; MacCraith, B. D.; McEvoy, A. K. *Anal. Chem.* **1998**, *70*, 45. (c) Stein, E. W.; Grant, P. S.; Zhu, H.; McShane, M. J. *Anal. Chem.* **2007**, *79*, 1339.

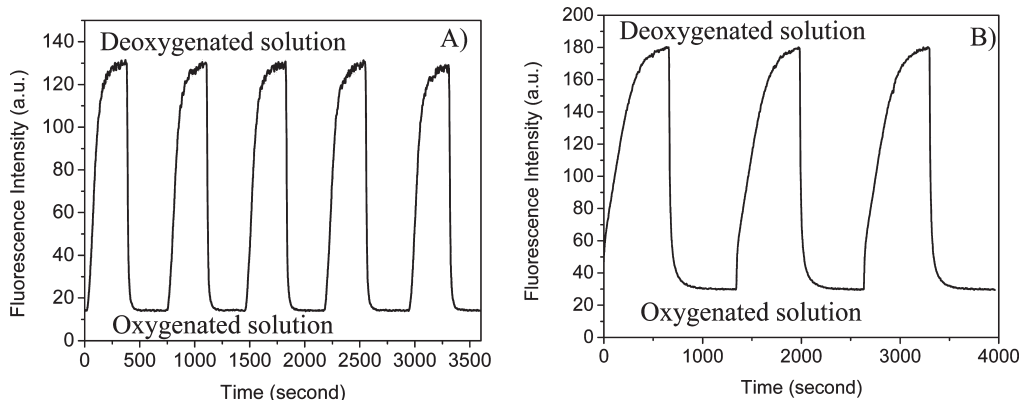

**Figure 4.** Response time of the film (A) F2 with covalently cross-linked **2** in PHEMA and (B) F6 with covalently cross-linked **2** in PS to deoxygenated solution using nitrogen gas and oxygenated solution using oxygen gas.

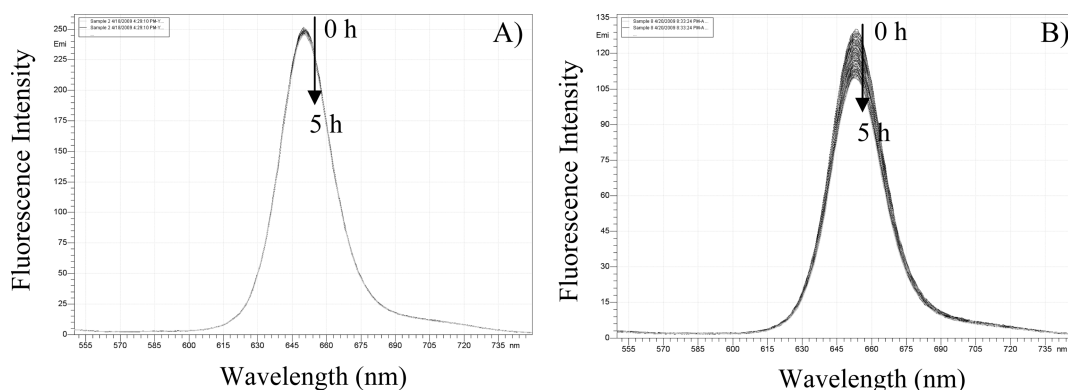

**Figure 5.** Photostability of (A) covalently cross-linked **2** in PHEMA (F2), and (B) physically doped PtTFPP in PHEMA (F4) in pH 7.0 B-R buffer with 5 h of continuous exposure at 405 nm ( $0.2 \text{ mW/cm}^2$ ).

1–2 min to DO. Therefore, the PHEMA hydrogel-based optical sensing film exhibits good response time (50 s for  $t_{95}$ ) to DO, enabling a new avenue for dissolved oxygen sensing. The response time can be even faster through a decrease in film thickness, an increase in the nitrogen/oxygen bubbling velocity of our setup (see Experimental Section for details), or a use of microspheres of the PHEMA gel dispersed in aqueous solution. For example, Borisov et al.<sup>18</sup> recently reported a fast DO response optical sensor (about 4 s) using polystyrene-*block*-polyvinylpyrrolidone beads with physically incorporated PtTFPP suspended in liquids.


**Photostability of the Sensing Membranes (F2 vs F4) in Aqueous Solutions.** Short-term photostability was studied in pH 7.0 B-R buffer using F2 and F4 at ambient air condition. The films were continuously exposed by excitation light at 405 nm ( $0.2 \text{ mW/cm}^2$ ) over a period of 5 h with 150 measurements. It was observed that F2 (Figure 5A) was quite stable under our experimental conditions with less than 1% total intensity decrease, which corresponded to a variation of less than 0.0067% per measurement. A dramatically different result was observed for F4 under the same experimental conditions, where 16% of total emission decay (Figure 5B) was observed corresponding to a decay of 0.11% per measurement.

The photostability study strongly indicated that chemical bonding of the sensors with their matrix could improve the sensors' photostability. It was pointed out by Lee et al.<sup>5</sup> that molecular movement in the sensor film is an important factor affecting the sensors' photostability. We believe the cross-linking of the sensors within the polymer matrices restricts the sensor molecules' movement and results in the sensors being less reactive toward photo-oxidation and reduction to increase their photostability as compared to the physically incorporated PtTFPP in the same matrices.

**Interference Tests for F2 Film.** As stated above, we successfully prepared the chemically bonded sensing films using the PHEMA hydrogel as the matrix and demonstrated that these new sensing films exhibited reasonable oxygen response, excellent photostability, nonleaching character, and good response time. The interference by ions, pH values, mediums, and temperature was further studied using the film F2.

Interference by ions, pH values, and amino acids in media often occur when the sensors are applied in various liquid environments. Interference is generally significantly reduced, but not always removed completely, upon the immobilization of sensor molecules in various polymer matrices. One mM NaCl, KCl, and CaCl<sub>2</sub> in the B-R pH 7 buffers, as well as varied pH values from 2 to 9, have no obvious influence on the emission intensity (with a

(18) Borisov, S. M.; Mayr, T.; Klimant, I. *Anal. Chem.* **2008**, *80*, 573.

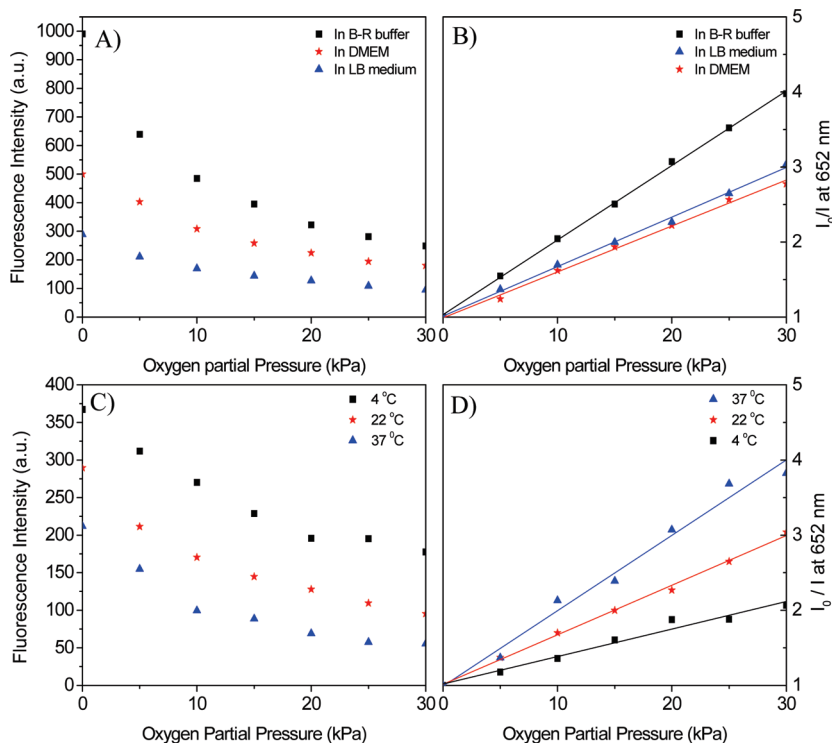

**Figure 6.** (A, B) Medium influence on the oxygen sensing at room temperature (22 °C) and (C, D) temperature effect on the oxygen sensing in LB medium. F2 film was used for this study. The fluorescence intensities at 652 nm were given in the left y-axis. Ratios of  $I_0/I$  were given in the right y-axis.  $I_0$  is the emission intensity in the deoxygenated buffer by flushing with nitrogen.  $I$  is the emission intensity of oxygen-containing solutions equilibrated at different oxygen partial pressures. Fitting of the Stern–Volmer plots (B, D) is performed using eq 1.

emission variation of less than 1%) as compound **2** is neutral and has no pH, sodium, potassium, or calcium ion-sensitive groups or ligands. On the contrary, Dulbecco's Modified Eagle's Medium (DMEM) and Lysogeny Broth medium (LB) have significant influence on the emission intensity. 30% fluorescence intensity decay in DMEM and 60% decay in LB medium were observed as compared to that in B-R buffer (Figure 6A), showing that combinations of salts, amino acids, vitamins, sugars, proteins, and extract of yeast present in the media likely interact with the sensors. Similar influences of LB medium in decreasing emission intensities of PtTFPP sensors dispersed in the polystyrene-*block*-polyvinylpyrrolidone beads were reported by Borisov et al.<sup>18</sup>

Media not only decreased the emission intensities as compared to that in B-R buffer, but also affected the oxygen responses. Figure 6A shows the emission intensities of the F2 film and Figure 6B gives Stern–Volmer fittings of the film in the three different aqueous solutions at the same oxygen partial pressures. It was found that the sensing film had the highest Stern–Volmer quenching effect in the B-R buffer and the lowest quenching effect in DMEM medium. Table 2 gives the detailed  $K_{SV}$  values. On the other hand, high-temperature decreased the sensor's fluorescence intensity (Figure 6C) but increased the oxygen quenching effect (Figure 6D), which is a common phenomenon for many oxygen sensors in thin films,<sup>14b,c</sup> most likely because of an enhanced interaction of the sensing moieties with oxygen molecules at high temperature. This indicates that when used for practical DO detection, careful calibration in the specific environment

**Table 2.** Stern–Volmer Quenching Constants ( $K_{SV}$  in  $\text{kPa}^{-1}$ ) of the Sensing Film F2 in B-R Buffer, DEME and LB Medium at 4, 22, and 37 °C<sup>a</sup>


temp	DMEM	LB medium	B-R buffer (pH 7.5)
37 °C	0.091 (0.971)	0.10 (0.984)	0.13 (0.975)
22 °C	0.061 (0.998)	0.066 (0.997)	0.088 (0.997)
4 °C	0.029 (0.990)	0.029 (0.989)	0.038 (0.964)

<sup>a</sup> Values in parentheses are the correlation coefficients ( $R^2$ ) of the Stern–Volmer fitting.

is necessary and the temperature should be controlled precisely to eliminate experimental error.

**Toxicity to Cells.** Toxicity to A549 cancer cells was investigated using F2 films evaluated by a 3-(4,5-dimethylthiazol-2-yl)-2,5-diphenyltetrazolium bromide (MTT) viability assay. The MTT assay is based on intracellular reduction of a tetrazolium dye to a formazan product measured spectrophotometrically, and is used for high-throughput screening.<sup>19</sup> No inhibition for cell proliferation or cytotoxicity was observed after 24 h of incubation of the cancer cells in the presence of the sensing membranes (Figure 7). The nontoxicity demonstrated a good biocompatibility of the new sensing membranes. Although the oxygen sensor contains the heavy metal platinum atom, it is chemically linked with the polymer matrix to prevent its leaching into the medium, which endows the sensing membranes to be nontoxic.

(19) (a) Mosmann, T. *J. Immun. Methods* **1983**, *65*, 55. (b) Carmichael, J.; Degraff, W. G.; Gazdar, A. F.; Minna, J. D.; Michell, J. B. *Cancer Res.* **1987**, *47*, 936.

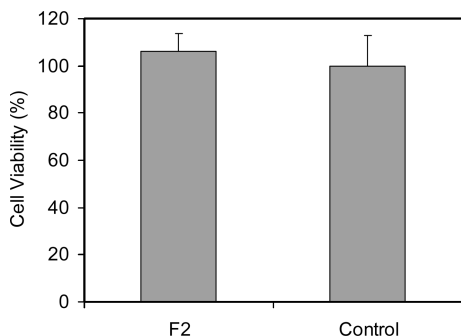

**Figure 7.** Viability (MTT) of A549 cells incubated in the presence of the sensing membrane F2 in DMEM for 24 h.

**Table 3.** DO ( $pO_2$  in kPa)<sup>a</sup> Determination Using Film F2 in B-R pH 7.5 Buffer<sup>b</sup>

set value	determined value <sup>c</sup>	difference in %
5.1	5.2 (+0.1)	+2.0
8.1	7.5 (-0.6)	-7.4
20.2	20.6 (+0.4)	+2.0
27.4	28.8 (+1.4)	+5.1

<sup>a</sup>  $pO_2$  represents the oxygen partial pressure in kPa. <sup>b</sup> Experiment performed at atmosphere pressure. <sup>c</sup> Values in the parentheses were the differences between the measured and set values.

**Storage Stability.** All of the sensing films can be stored in the dark at room temperature for at least 6 months. Because of the nonleaching character of the chemically conjugated sensing membranes, the films of **2** in PHEMA and PS matrices can be stored in aqueous solution for at least 3 months without alteration of their sensing performances.

**Validation.** The oxygen response functions were tested in pH 7.5 buffers equilibrated with oxygen and nitrogen gas mixtures with 5, 8, 20, and 27% of oxygen corresponding to  $pO_2$  of 5.1, 8.1, 20.2, and 27.4 kPa using F2 film. Experiments were performed at room temperature. The tested results are given in Table 3. The numbers in the parentheses in the table are the differences from the measured values and the adjusted values of the tested solutions. It can be seen that the sensing films gave good DO determinations not exceeding  $\pm 7.4\%$  of the set values.

### 3. Conclusion

A new oxygen sensor was successfully prepared through a simple chemical modification of the popularly used oxygen sensor PtTFPP. Using the reactivity of methacrylate active groups, the new sensor was able to be chemically embedded into hydrophilic PHEMA and hydrophobic PS for dissolved oxygen sensing studies. Physically incorporated PtTFPP, which is the precursor of the new sensor, in the same PHEMA and PS was also evaluated as a counterpart for a demonstration of the advantages of the chemically conjugated approach. Results showed that the chemically bonded sensors (i) alleviated the leaching problem of the sensors from their matrices and (ii) improved sensors' photostability. It was also demonstrated that the biocompatible PHEMA gel is a good matrix for oxygen

sensing, because the ability for dissolved oxygen to diffuse in the PHEMA matrix is significantly larger than that in the PS matrix, resulting in faster response time and higher oxygen sensitivity for dissolved oxygen in the PHEMA matrix than in the hydrophobic PS matrix. pH values did not interfere with the sensors. However, the media (LB and DMEM) had influences on the emission intensity and response to oxygen, suggesting that the components in the media (protein, amino acids, sugar, and/or yeast extract) likely interact with the sensor molecules. Temperature is critical in affecting the quenching velocity. Higher temperature results in a faster quenching velocity although the emission intensity decreases.

Thus, we have studied new hydrophilic PHEMA hydrogel-based oxygen sensing films in detail. We have also demonstrated the advantages of the chemically cross-linked oxygen sensor films. It is expected that using the cross-linking method to chemically conjugate oxygen sensor molecules to the biocompatible hydrophilic matrix will provide a new avenue to broaden the oxygen sensor's applications in biological fields. Using the sensing film, which is biocompatible and suitable as a 3D scaffold for tissue engineering, for more understanding of cell growth, proliferation, and metabolism is expected and in progress.

## 4. Experimental Section

**4.1. Materials and Reagents.** All chemicals and solvents were of analytical grade and were used without further purifications. Anhydrous ethylene glycol, sodium hydride (NaH), methacryloyl chloride, *N,N'*-dimethyl formamide (DMF), trimethylsilylpropyl acrylate (TMSPA), styrene, HEMA, azobisisobutyronitrile (AIBN), and acrylamide were commercially available from Aldrich and used without further purification. Ethyloxy-lylate trimethylolpropane triacrylate (SR454) was a commercial product of Sartomer Company (Exton, PA). PtTFPP was commercially available from Frontier Scientific Inc. (Logan, UT). Doubly distilled water was used for the preparation of the buffer solutions. The pH values were determined with a digital pH meter (Thermo Electron Corporation, Beverly, MA) calibrated at room temperature ( $23 \pm 2^\circ\text{C}$ ) with standard buffers of pH 10.01, 7.00, and 4.01. Britton-Robinson (B-R) buffers composed of acetic acid, boric acid, phosphoric acid, and sodium hydroxide were used for tuning pH values. Calibration gases (nitrogen and oxygen, each of 99.999% purity) were purchased from AIR Liquide America, LP (Houston, TX). Exact gas percentage was controlled using a homemade gas manipulator. All measurements of sensing behaviors were carried out at atmospheric pressure (760 mmHg, or 101 kPa) at room temperature ( $23 \pm 2^\circ\text{C}$ ) unless specified. Quartz glass from University Wafer (South Boston, MA) was cut into squares of  $1.31\text{ cm} \times 1.31$  and  $0.36\text{ cm} \times 0.36$  cm using a dicer (Micro-automation, Billerica, MA) for fluorescence measurement. DMEM was purchased from Invitrogen (Carlsbad, California). LB medium was made of 10 g tryptone, 5 g yeast extract, and 10 g NaCl in 1 L distilled water.

**4.2. Instruments.** Varian liquid-state NMR operated at 400 MHz for  $^1\text{H}$  NMR, 100 MHz for  $^{13}\text{C}$  NMR, and 376 MHz for  $^{19}\text{F}$  NMR were used for spectra measurements. Matrix assisted laser desorption/ionization time-of-flight (MALDI-TOF) mass spectrometry was performed by the ASU Mass Spectrometry



Laboratory. An oxygen plasma cleaner (Harrick Plasma, Ithaca, NY) was used for quartz glass surface activation. Shimadzu RF-5301 spectrofluorophotometer (Shimadzu Scientific Instruments, Columbia, MD) was used for fluorescence measurements. For an easy measurement of the films in liquid solutions, the quartz glass was cut with a dicer into squares of 1.31 cm × 1.31 cm, which can fit diagonally into quartz fluorescence cuvettes to enable the sensing membrane be positioned at an angle of 45° to the excitation light. Contact angle measurements were made using an FTA 1000C instrument (NanoDispense Inc., Fremont, CA). Temperature was adjusted from 20 to 37 °C using a Fisher Scientific Isotemp 202S water bath with a temperature variation accuracy of ±0.5 °C.

**4.3. Quartz Substrate Modification Using TMSPA.** To achieve stable polymer membranes on the quartz glasses, the quartz surface was modified with TMSPA. Detergent and acetone-cleaned quartz glass was treated with oxygen plasma for ~30 min to generate active hydroxyl groups. Immediately following plasma treatment, the quartz glass was placed in a vacuum chamber to graft a thin layer of TMSPA on its surface under vacuum for 20 h using a known vapor deposition approach.<sup>8</sup>

**4.4. Preparation of PHEMA Polymer Membranes.** 0.1 mg, 1 mg, or 10 mg of the sensor monomer **2** or PtTFPP, HEMA (800 mg), acylamide (150 mg), SR454 (50 mg), and AIBN (10 mg) were dissolved in 1 mL of DMF as stock solutions. Ten microliters of the stock solution were added onto the surface of the TMSPA-modified quartz glass and covered with a clean but untreated coverslip to make a sandwich structure. The thickness was controlled using 25 μm Kapton tape (DuPont, Wilmington, DE). The sandwich setup was placed into a vacuum oven, which was evacuated and refilled with nitrogen three times. Polymerization was carried out under nitrogen at 80 °C for 1.5 h in the oven. The quartz glasses with polymer membranes were removed from the oven, with Kapton tape and nonsurface modified glass being removed from the polymerized membrane surface. The uniform polymer membranes on the quartz glasses were washed three times using methanol to remove any remaining nonpolymerized monomers and residual DMF. The films were dried and stored in the dark at room temperature.

**4.5. Preparation of PS Polymer Membranes.** The preparation of the PS polymer membranes was similar to that of PHEMA; however, styrene was used instead of HEMA and acrylamide.

**4.6. Release Study.** The sensor membranes were immersed in the B-R pH 7.5 buffer and methanol for a certain time. Spectra were taken under the same optical setup as before. To test whether there is any sensors' emission in the buffer or methanol, was took out the sensing film from the cuvette and measured the emission of the liquids.

**4.7. Photostability Study.** The sensing membranes in pH 7.0 B-R buffer were continuously exposed by excitation light at 405 nm (0.2 mW/cm<sup>2</sup>) over a period of 5 h. The membrane fluorescence intensity was recorded with an interval of 2 min.

**4.8. Response Time Study.** Sensing films were placed diagonally into a quartz cuvette with approximately 2 mL of B-R buffer (pH 7). Emission measurements were taken every 4 s at the sensor's peak emission at 650 nm excited at 405 nm. To vary the concentration of dissolved oxygen in the buffers, we used a gas manifold to control gas flow through a tube and needle to bubble the buffer. Holes were installed in the cuvette cap to allow the needle into the cuvette and gas flow out. The needle was positioned so the bubbling would occur in the buffer just above the sensor film to decrease the possible interference by the gas bubbles, which may affect the fluorescence measurements. Oxygen and nitrogen flow rates were set at 66 standard cubic

centimeters per minute. In all trials, the buffer was first saturated with oxygen before beginning the measurements. Measurements began with the change from 100% oxygen flow into the buffer to 100% nitrogen, and then continued as the gas flow composition was switched between oxygen and nitrogen. The intervals of gas flow depended on the type of film. For the PHEMA films, 360 s was the interval for nitrogen and oxygen bubbling; for the PS films, 660 s was used as the interval.

**4.9. MTT Assay for Cytotoxicity Study.** The assay was performed by an in vitro MTT-based toxicology assay kit (Sigma). A549 cancer cells (American Type Culture Collection (ATCC), Manassas, VA) were cultured in DMEM supplemented with 10% fetal bovine serum, 5% penicillin, and 2 mM L-glutamine (Sigma) and were incubated at 37 °C in a 5% CO<sub>2</sub> atmosphere. The cells were seeded onto 96-well plates at 10 000 cells per well, and incubated for 1 day. The sensing membranes (0.36 cm × 0.36 cm) on the quartz glasses were immersed into the DMEM growth medium and the cells with the sensing membranes were incubated in the 96 well plates. Twenty-four hours later, the membranes were removed from the 96-well plates. The medium in the wells were removed and the cells were washed with PBS buffer and then incubated in fresh DMEM medium (100 μL) and 10 μL of MTT solution (5 mg/mL) in 5% CO<sub>2</sub> at 37 °C for another 3 h. Sixty microliters of the culture medium was removed and 50 μL of DMSO was added to each well to dissolve the internalized purple formazan crystals by gentle pipetting up and down. The absorbance was measured at a wavelength of 490 nm using SpectraMax 190 from Molecular Devices (Downingtown, PA). Each experiment was conducted twice in triplicate. The result was expressed as a percentage of the absorbance of the blank control.

**4.10. Synthesis of Compound 1.** 180 mg of 40% NaH oil (3 mmol) was added to a solution of 2.2 g of ethylene glycol (35.48 mmol) in 30 mL of dry THF. The mixture was stirred at room temperature for 30 min, and then PtTFPP (720 mg, 0.63 mmol) was added in one portion. The mixture was stirred at room temperature for 24 h to complete the reaction. After THF was removed, the residue was poured into sodium chloride solutions. The product was extracted into ethyl acetate, dried over Na<sub>2</sub>SO<sub>4</sub>, and purified using column chromatography with chloroform/methanol (10:1 by volume) to get 600 mg of compound **1**. Yield: 71%. <sup>1</sup>H NMR: (400 MHz, CD<sub>3</sub>COCD<sub>3</sub>, δ ppm) 9.21 (s, 8H), 4.68 (t, 8H), 4.23 (m, 4H), 4.08 (t, 8H). <sup>13</sup>C NMR (100 MHz, CD<sub>3</sub>COCD<sub>3</sub>, δ in ppm): 150.53, 148.10, 145.35, 144.30, 142.89, 142.75, 134.29, 115.29, 115.09, 114.90, 109.88, 79.62, 63.80. <sup>19</sup>F-NMR (376 MHz, CD<sub>3</sub>COCD<sub>3</sub>, δ in ppm, CF<sub>3</sub>COOH = -76.55 ppm): -136.96 (8F, dd, J<sub>F-F</sub> = 14 Hz, J<sub>F-F</sub> = 28 Hz), -153.29 (8F, dd, J<sub>F-F</sub> = 14 Hz, J<sub>F-F</sub> = 28 Hz). MALDI-TOF-Mass: C<sub>52</sub>H<sub>29</sub>N<sub>4</sub>O<sub>8</sub>F<sub>16</sub>Pt: calcd, 1335.85; measured, 1335.16.

**4.11. Synthesis of Compound 2.** Compound **1** (50 mg, 0.037 mmol) and 300 mg triethylamine (2.97 mmol) were dissolved in 5 mL of DMF and cooled to 0 °C. To this solution was slowly added 100 μL (~108 mg, 1.0 mmol) of methacryloyl chloride in 500 μL of THF. The mixture was stirred at room temperature overnight. Thin layer chromatography (TLC) was used to verify that the reaction was completed. The mixture was poured into water. Organic product was extracted into ethyl acetate and dried over Na<sub>2</sub>SO<sub>4</sub>. After the ethyl acetate was removed, the residue was washed with hot methanol twice and filtered to yield 40 mg of sensor **2** with a yield of 64%. <sup>1</sup>H NMR (400 MHz, DMSO-d<sub>6</sub>, δ ppm): 9.22 (s, 8H), 6.16 (s, 4H), 5.79 (s, 4H), 4.82 (t, 8H), 4.60 (t, 8H), 1.96 (s, 12H). <sup>13</sup>C NMR (100 MHz, DMSO-d<sub>6</sub>, δ in ppm): 166.93, 147.66, 145.28, 142.78, 141.49, 140.29, 138.77,

136.20, 132.56, 126.65, 112.73, 112.53, 107.09, 73.59, 64.10, 18.40.  $^{19}\text{F}$ -NMR (376 MHz, DMSO- $d_6$ ,  $\delta$  in ppm,  $\text{CF}_3\text{COOH} = -76.55$  ppm):  $-141.11$  (8F, d,  $J_{\text{F-F}} = 18$  Hz),  $-156.91$  (8F, d,  $J_{\text{F-F}} = 18$  Hz).

**Acknowledgment.** This work was supported by a grant from the NIH National Human Genome Research Institute, Centers of Excellence in Genomic Science, Grant 5 P50 HG002360. We also thank Dr. Yongzhong Li at Center for

Ecogenomics for the evaluation of the toxicity of the sensor films.

**Supporting Information Available:** Pictures of a typical thin film absorbance and emission spectra of PtTFPP, compound **1**, and compound **2** in THF solutions, and the photostability of PtTFPP in 5% THF-containing B-R 7 buffer (PDF). This material is available free of charge via the Internet at <http://pubs.acs.org>.