


Development of a Functionalized Xenon Biosensor

Megan M. Spence, E. Janette Ruiz, Seth M. Rubin, Thomas J. Lowery,
Nicolas Winssinger, Peter G. Schultz, David E. Wemmer, and Alexander Pines

J. Am. Chem. Soc., **2004**, 126 (46), 15287-15294 • DOI: 10.1021/ja0483037 • Publication Date (Web): 29 October 2004

Downloaded from <http://pubs.acs.org> on April 5, 2009

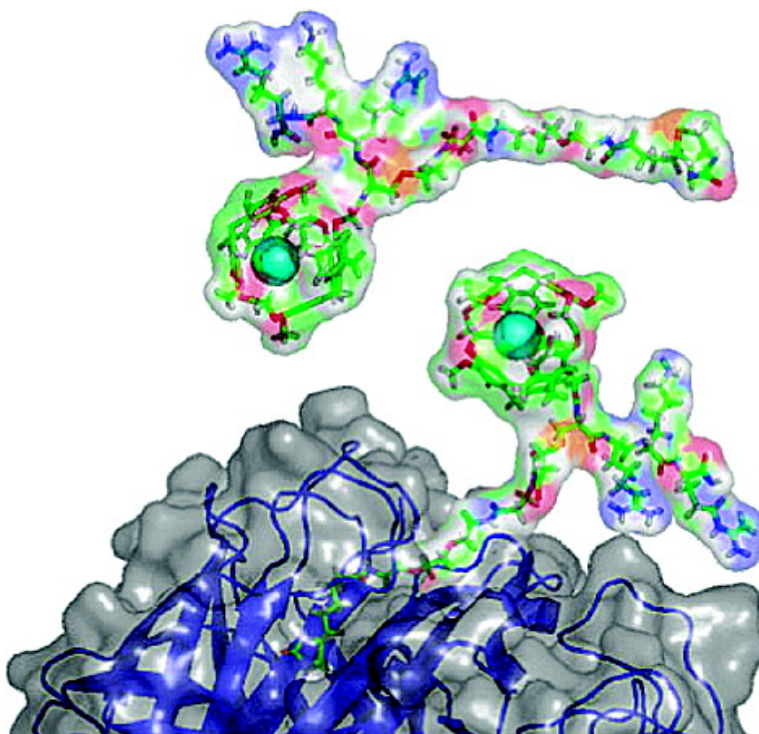

More About This Article

Additional resources and features associated with this article are available within the HTML version:

- Supporting Information
- Links to the 9 articles that cite this article, as of the time of this article download
- Access to high resolution figures
- Links to articles and content related to this article
- Copyright permission to reproduce figures and/or text from this article



[View the Full Text HTML](#)



Development of a Functionalized Xenon Biosensor

Megan M. Spence,^{†,‡,⊥} E. Janette Ruiz,^{†,‡} Seth M. Rubin,^{†,§,#} Thomas J. Lowery,^{†,§}
Nicolas Winssinger,^{||,+} Peter G. Schultz,^{||} David E. Wemmer,^{†,§} and
Alexander Pines^{*,†,‡}

Contribution from the Department of Chemistry, University of California at Berkeley, Berkeley, California 94720, Materials Sciences and Physical Biosciences Divisions, Lawrence Berkeley National Laboratory, Berkeley, California 94720, and Department of Chemistry and the Skaggs Institute for Chemical Biology, The Scripps Research Institute, 10550 North Torrey Pines Road, La Jolla, California 92037

Received March 24, 2004; E-mail: pines@berkeley.edu

Abstract: NMR-based biosensors that utilize laser-polarized xenon offer potential advantages beyond current sensing technologies. These advantages include the capacity to simultaneously detect multiple analytes, the applicability to in vivo spectroscopy and imaging, and the possibility of “remote” amplified detection. Here, we present a detailed NMR characterization of the binding of a biotin-derivatized caged-xenon sensor to avidin. Binding of “functionalized” xenon to avidin leads to a change in the chemical shift of the encapsulated xenon in addition to a broadening of the resonance, both of which serve as NMR markers of ligand–target interaction. A control experiment in which the biotin-binding site of avidin was blocked with native biotin showed no such spectral changes, confirming that only specific binding, rather than nonspecific contact, between avidin and functionalized xenon leads to the effects on the xenon NMR spectrum. The exchange rate of xenon (between solution and cage) and the xenon spin–lattice relaxation rate were not changed significantly upon binding. We describe two methods for enhancing the signal from functionalized xenon by exploiting the laser-polarized xenon magnetization reservoir. We also show that the xenon chemical shifts are distinct for xenon encapsulated in different diastereomeric cage molecules. This demonstrates the potential for tuning the encapsulated xenon chemical shift, which is a key requirement for being able to multiplex the biosensor.

Introduction

Developments of new approaches in analytical chemistry are being increasingly driven by advances and applications of combinatorial chemistry and parallel assays. Products of combinatorial syntheses require fast and sensitive screening techniques due to the production of large numbers of chemical analogues to be tested for affinity, catalytic activity, or other properties of interest.^{1–3} Various detection methodologies for high-throughput screening (HTS) applications, including laser-induced fluorescence, fluorescence polarization, and fluorescence energy transfer, have been implemented in high-density microtiter plate format.^{4–7} The spatial separation of possible

interacting pairs distinguishes signals from different ligand–target combinations, and readings are made by scanning techniques or by imaging.⁸ At present, particular challenges exist in the development of multiplexed assays, which allow multiple interactions in samples to be detected simultaneously.

Macromolecule-based biosensors exploit the specificity and strength of biological ligand–target interactions to selectively signal the presence of particular molecular targets. These biosensors rely on the coupling of biological recognition events to an experimental observable, allowing external detection. Historically, biosensors have been used for routine analyses in clinical diagnosis, as in the case of the traditional glucose sensor;⁹ however, new concepts in biosensor design are being considered for high-throughput applications such as drug discovery.¹⁰ Recent developments in biosensor technology, such as surface plasmon resonance chips,¹¹ are already being developed in a multiplexed format.¹²

Nuclear magnetic resonance (NMR) is powerful in analytical chemistry applications due to its high information content. Steady progress is being made to incorporate NMR analysis

[†] University of California at Berkeley.

[‡] Materials Sciences Division, Lawrence Berkeley National Laboratory.

[§] Physical Biosciences Division, Lawrence Berkeley National Laboratory.

^{||} The Scripps Research Institute.

[⊥] Current address: ETH-Zürich, Laboratorium für Physikalische Chemie, CH-8093 Zürich, Switzerland.

[#] Current address: Memorial Sloan-Kettering Cancer Center, 1275 York Avenue, New York, NY 10021.

⁺ Current address: ISIS, Louis Pasteur University, 8 allée Gaspard Monge, F-67000 Strasbourg, France.

(1) Hogan, J. C. *Nature* **1996**, *384*, 17–19.

(2) Cawse, J. N. *Acc. Chem. Res.* **2001**, *34*, 213–221.

(3) Lehn, J. M.; Eliseev, A. V. *Science* **2001**, *291*, 2331–2332.

(4) Checovich, W. J.; Bolger, R. E.; Burke, T. *Nature* **1995**, *375*, 254–256.

(5) Broach, J. R.; Thorne, J. *Nature* **1996**, *384*, 14–16.

(6) Gauglitz, G. *Curr. Opin. Chem. Biol.* **2000**, *4*, 351–355.

(7) Khandurina, J.; Guttman, A. *Curr. Opin. Chem. Biol.* **2002**, *6*, 359–366.

(8) Cheung, V. G.; Morley, M.; Aguilar, F.; Massimi, A.; Kucherlapati, R.; Childs, G. *Nat. Genet.* **1999**, *21*, 15–19.

(9) Ziegler, C.; Gopel, W. *Curr. Opin. Chem. Biol.* **1998**, *2*, 585–591.

(10) Keusgen, M. *Naturwissenschaften* **2002**, *89*, 433–444.

(11) Malmqvist, M. *Nature* **1993**, *361*, 186–187.

(12) Johnston, K. S.; Mar, M.; Yee, S. S. *Sens. Actuators, B* **1999**, *54*, 57–65.

into high-throughput and combinatorial chemistry applications.^{13–18} Utilization of conventional NMR for high-throughput biosensor applications may be limited by the intrinsically low sensitivity and the complexity of spectra obtained from biomolecules and mixtures. Laser-polarization¹⁹ of ¹²⁹Xe offers an increase in signal-to-noise by several orders of magnitude relative to the equilibrium nuclear-spin polarizations measured in normal NMR experiments.^{20,21} In addition, ¹²⁹Xe NMR spectra are less complex than those from ¹H or ¹³C NMR, usually showing only a few, easily interpretable lines with no background signal. Despite its spectral simplicity, xenon exhibits the important property that it can sensitively report on its local environment via its chemical shift and relaxation parameters. Furthermore, xenon NMR and MRI can take advantage of “remote” detection of signals that can be used to reconstruct substantially amplified spectra²² and images.²³ NMR of ¹²⁹Xe has been used to investigate the structure and dynamics of materials,^{24–27} molecular cages,^{28–34} biological systems, and for biomedical applications.^{35–37} Recently, extensive reviews regarding the history and development of hyperpolarized xenon NMR have been published.^{38,39}

Biological systems studied with ¹²⁹Xe NMR include globular proteins such as myoglobin and hemoglobin,^{40–46} membrane associated peptides such as gramicidin,⁴⁷ and lipid membranes

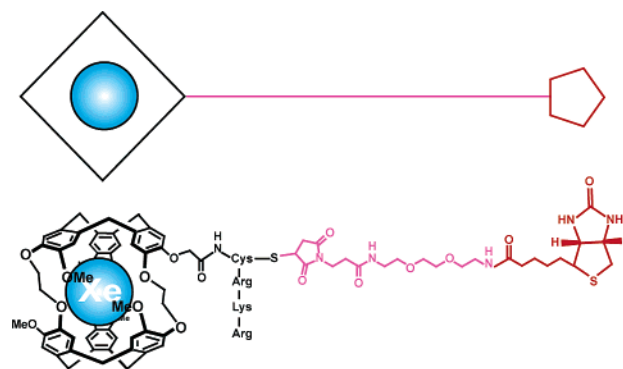


Figure 1. Structure and schematic representation of biosensor molecule designed target xenon to avidin with high affinity and specificity. Cryptophane-A (black) binds the xenon atom, and the biotin ligand (red) is connected to encapsulated xenon via a linker (purple).

themselves.⁴⁸ While xenon shows appreciable binding to many proteins, as evidenced by its use in making heavy atom derivatives of protein crystals for X-ray crystallography,^{49,50} the xenon-protein binding constants are relatively low ($K_a \approx 10\text{--}100\text{ M}^{-1}$). The exchange of bound and free xenon has been found to be fast on the time-scale of the chemical shift difference between the protein and solvent environments, leading to NMR spectra with a single xenon resonance. The chemical shift reflects a population-weighted average over the xenon chemical shifts of the available environments: solvent, protein interior, and protein surface. As a result, the chemical shift value of this single peak can report on changes in protein interactions. Experiments with maltose binding protein demonstrated that the ¹²⁹Xe chemical shift responds to a change in protein conformation upon ligand binding; the difference in shift results from distinct xenon-protein interactions between the two conformers.^{44,45} However, to induce measurable shifts, relatively high concentrations of the “analyte” are required.

Despite the favorable attributes of xenon interacting with proteins in solution, high-sensitivity molecular sensing is not compatible with the fast-exchange characteristic of xenon-protein interactions. This limitation can be overcome by identifying xenon interactions that report analyte binding via a unique resonance that is resolved from those averaged into the single fast-exchange peak. To realize this, we have taken the approach of “functionalizing” the xenon by providing a physical coupling between xenon and the ligand that targets a protein. Recently, as a proof-of-principle case, we reported a molecule designed to be an NMR biosensor that targeted the biotin-binding protein avidin.⁵¹ The sensor consists of a modified cryptophane-A cage, to which xenon binds as the NMR reporter,

- (13) Shuker, S. B.; Hajduk, P. J.; Meadows, R. P.; Fesik, S. W. *Science* **1996**, *274*, 1531–1534.
- (14) Keifer, P. A. *Curr. Opin. Biotechnol.* **1999**, *10*, 34–41.
- (15) Lacey, M. E.; Subramanian, R.; Olson, D. L.; Webb, A. G.; Sweedler, J. V. *Chem. Rev.* **1999**, *99*, 3133–3152.
- (16) Shapiro, M. J.; Gounarides, J. S. *Prog. Nucl. Magn. Reson. Spectrosc.* **1999**, *35*, 153–200.
- (17) Olson, D. L.; Peck, T. L.; Webb, A. G.; Magin, R. L.; Sweedler, J. V. *Science* **1995**, *270*, 1967–1970.
- (18) Hou, T.; Smith, J.; MacNamara, E.; Macnaughtan, M.; Raftery, D. *Anal. Chem.* **2001**, *73*, 2541–2546.
- (19) Happer, W. *Rev. Mod. Phys.* **1972**, *44*, 169–249.
- (20) Walker, T. G.; Happer, W. *Rev. Mod. Phys.* **1997**, *69*, 629–642.
- (21) Zook, A. L.; Adhyaru, B. B.; Bowers, C. R. *J. Magn. Reson.* **2002**, *159*, 175–182.
- (22) Moule, A. J.; Spence, M. M.; Han, S. I.; Seeley, J. A.; Pierce, K. L.; Saxena, S.; Pines, A. *Proc. Natl. Acad. Sci. U.S.A.* **2003**, *100*, 9122–9127.
- (23) Seeley, J. A.; Han, S. I.; Pines, A. *J. Magn. Reson.* **2003**, *167*, 282–290.
- (24) Ripmeester, J. A.; Ratcliffe, C. I.; Tse, J. S. *J. Chem. Soc., Faraday Trans. 1* **1988**, *84*, 3731–3745.
- (25) Chmelka, B. F.; Raftery, D.; McCormick, A. V.; Demenoral, L. C.; Levine, R. D.; Pines, A. *Phys. Rev. Lett.* **1991**, *66*, 580–583.
- (26) Springuel-Huet, M. A.; Bonardet, J. L.; Gedeon, A.; Fraissard, J. *Magn. Reson. Chem.* **1999**, *37*, S1–S13.
- (27) Sozzani, P.; Comotti, A.; Simonutti, R.; Meersmann, T.; Logan, J. W.; Pines, A. *Angew. Chem., Int. Ed.* **2000**, *39*, 2695–2698.
- (28) Cram, D. J.; Tanner, M. E.; Knobler, C. B. *J. Am. Chem. Soc.* **1991**, *113*, 7717–7727.
- (29) Bartik, K.; Luhmer, M.; Heyes, S. J.; Ottinger, R.; Reisse, J. *J. Magn. Reson., Ser. B* **1995**, *109*, 164–168.
- (30) Branda, N.; Grotzfeld, R. M.; Valdes, C.; Rebek, J. *J. Am. Chem. Soc.* **1995**, *117*, 85–88.
- (31) Bartik, K.; Luhmer, M.; Dutasta, J. P.; Collet, A.; Reisse, J. *J. Am. Chem. Soc.* **1998**, *120*, 784–791.
- (32) Syamala, M. S.; Cross, R. J.; Saunders, M. *J. Am. Chem. Soc.* **2002**, *124*, 6216–6219.
- (33) El Haouaj, M.; Luhmer, M.; Ko, Y. H.; Kim, K.; Bartik, K. *J. Chem. Soc., Perkin Trans. 2* **2001**, 804–807.
- (34) Song, Y. Q.; Goodson, B. M.; Taylor, R. E.; Laws, D. D.; Navon, G.; Pines, A. *Angew. Chem., Int. Ed. Engl.* **1997**, *36*, 2368–2370.
- (35) Albert, M. S.; Cates, G. D.; Driehuys, B.; Happer, W.; Saam, B.; Springer, C. S.; Wishnia, A. *Nature* **1994**, *370*, 199–201.
- (36) Albert, M. S.; Schepkin, V. D.; Budinger, T. F. *J. Comput. Assist. Tomogr.* **1995**, *19*, 975–978.
- (37) Albert, M. S.; Balamore, D. *Nucl. Instrum. Methods A* **1998**, *402*, 441–453.
- (38) Cherubini, A.; Bifone, A. *Prog. Nucl. Magn. Reson. Spectrosc.* **2003**, *42*, 1–30.
- (39) Goodson, B. M. *J. Magn. Reson.* **2002**, *155*, 157–216.
- (40) Miller, K. W.; Reo, N. V.; Uiterkamp, A. J. M. S.; Stengle, D. P.; Stengle, T. R.; Williamson, K. L. *Proc. Natl. Acad. Sci. U.S.A.* **1981**, *78*, 4946–4949.
- (41) Tilton, R. F.; Kuntz, I. D. *Biochemistry* **1982**, *21*, 6850–6857.
- (42) Rubin, S. M.; Spence, M. M.; Goodson, B. M.; Wemmer, D. E.; Pines, A. *Proc. Natl. Acad. Sci. U.S.A.* **2000**, *97*, 9472–9475.

- (43) Locci, E.; Dehouck, Y.; Casu, M.; Saba, G.; Lai, A.; Luhmer, M.; Reisse, J.; Bartik, K. *J. Magn. Reson.* **2001**, *150*, 167–174.
- (44) Rubin, S. M.; Spence, M. M.; Dimitrov, I. E.; Ruiz, E. J.; Pines, A.; Wemmer, D. E. *J. Am. Chem. Soc.* **2001**, *123*, 8616–8617.
- (45) Rubin, S. M.; Lee, S. Y.; Ruiz, E. J.; Pines, A.; Wemmer, D. E. *J. Mol. Biol.* **2002**, *322*, 425–440.
- (46) Bowers, C. R.; Storhaug, V.; Webster, C. E.; Bharatam, J.; Cottone, A.; Gianna, R.; Betsey, K.; Gaffney, B. J. *J. Am. Chem. Soc.* **1999**, *121*, 9370–9377.
- (47) Mckim, S.; Hinton, J. F. *Bba-Biomembranes* **1994**, *1193*, 186–198.
- (48) Xu, Y.; Tang, P. *Bba-Biomembranes* **1997**, *1323*, 154–162.
- (49) Schiltz, M.; Prange, T.; Fourme, R. *J. Appl. Crystallogr.* **1994**, *27*, 950–960.
- (50) Soltis, S. M.; Stowell, M. H. B.; Wiener, M. C.; Phillips, G. N.; Rees, D. C. *J. Appl. Crystallogr.* **1997**, *30*, 190–194.
- (51) Spence, M. M.; Rubin, S. M.; Dimitrov, I. E.; Ruiz, E. J.; Wemmer, D. E.; Pines, A.; Yao, S. Q.; Tian, F.; Schultz, P. G. *Proc. Natl. Acad. Sci. U.S.A.* **2001**, *98*, 10654–10657.

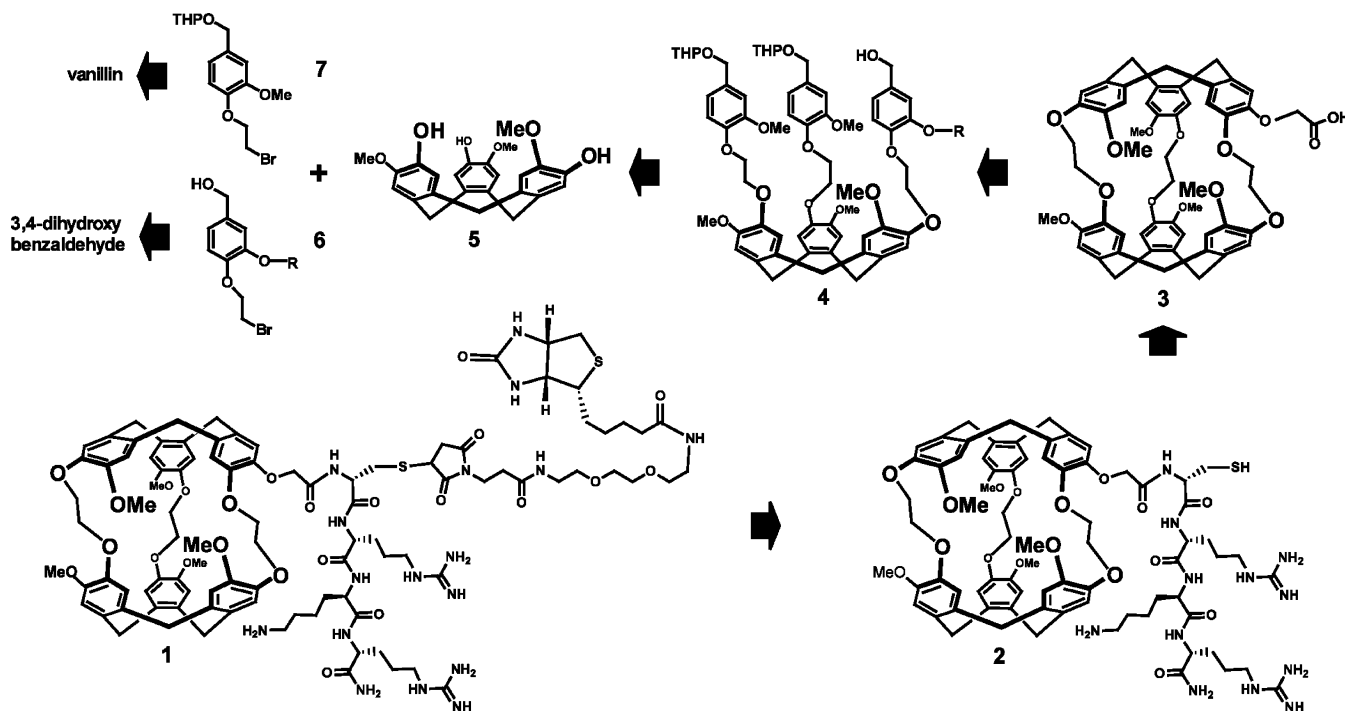


Figure 2. Retrosynthesis of the xenon biosensor.

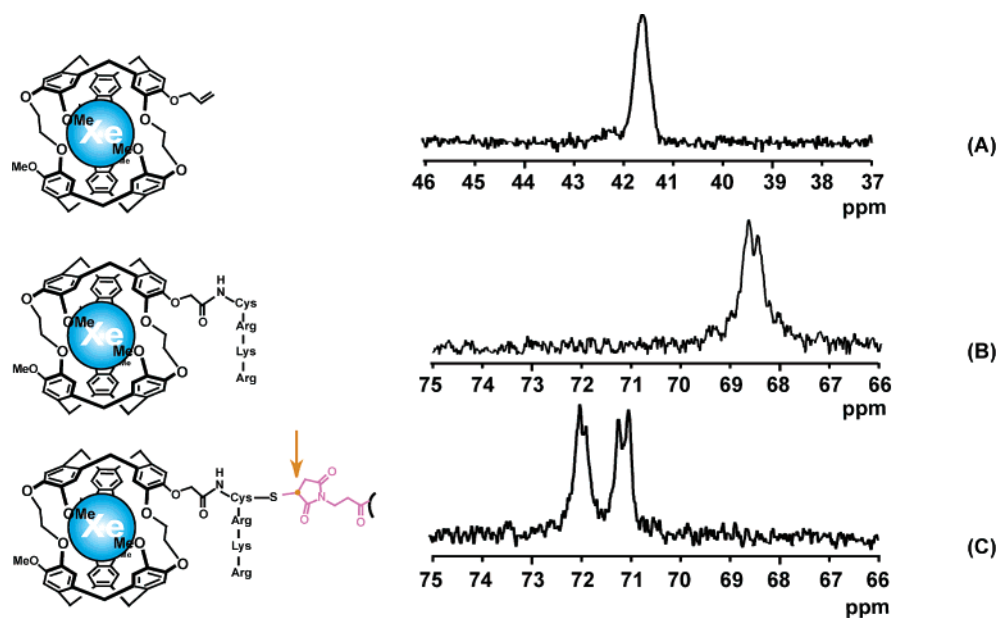


Figure 3. Detection of cage diastereomers by xenon chemical shift. The laser-polarized xenon spectrum of allyl-substituted cryptophane-A in 25% toluene/75% tetrachloroethane shows only one peak, with a line-width of 0.2 ppm (A). The addition of a single-enantiomer peptide chain to the cage leads to two xenon resonances (B), separated by ~ 0.10 ppm. The xenon spectrum after the addition of a biotin linker shows four lines (C), reflecting the effect of a racemic mixture at a chiral carbon seven bonds away from the cage itself.

connected via a tether to the ligand biotin (Figure 1). The ^{129}Xe NMR signal demonstrated a response to the binding of the sensor to avidin in solution. The stronger binding of xenon to cryptophane-A is associated with slow exchange as compared to the chemical shift difference between water and cryptophane-A environments; therefore, the resonance for functionalized xenon is distinct from xenon in bulk solution. The directly tethered ligand can bind to its target, with the bound xenon acting as a reporter (sensor) of this event through changes in its chemical shift and line width. The potential for multiplexed detection comes from the large ^{129}Xe chemical shift range of different cryptophanes. For example, increasing the length of

the methylene bridges by one carbon in cryptophane-A to make cryptophane-E leads to a ^{129}Xe chemical shift change of 30 ppm, implying that many versions with distinct chemical shifts can be made.⁵¹ Implementation of high-sensitivity fluorescence-based systems in a direct multiplexing assay is challenging due to spectral overlap, despite the high wavelength tunability of some systems such as quantum-dot-tagged microbeads.^{52,53} In microarray format, realization of the xenon biosensor could

(52) Han, M. Y.; Gao, X. H.; Su, J. Z.; Nie, S. *Nat. Biotechnol.* **2001**, *19*, 631–635.

(53) Nicewarmer-Pena, S. R.; Freeman, R. G.; Reiss, B. D.; He, L.; Pena, D. J.; Walton, I. D.; Cromer, R.; Keating, C. D.; Natan, M. J. *Science* **2001**, *294*, 137–141.

result in a high-density assay in which each well of the microtiter plate would not contain individual interacting pairs, but rather a single analyte interacting with a complete set of xenon biosensors, each consisting of a unique cage tethered to a unique targeting molecule. Within each well, binding to different targets would be distinguishable on the basis of chemical shift.

In this work, we provide a detailed characterization of this avidin binding, functionalized xenon system. The high sensitivity of the functionalized xenon to its environment is demonstrated by the observation that different diastereomer products of the cryptophane synthesis yield different chemical shifts. Upon the addition of protein, additional resonances appear in the spectrum that can be attributed to protein-bound functionalized xenon. An increase in the functionalized xenon resonance line width is apparent in the spectrum upon binding to the protein. The exchange rates of both protein-bound and free functionalized xenon were measured to investigate the origin of broadening in the protein-bound functionalized xenon resonance. Finally, two methods for signal-to-noise amplification by selective excitation of bound xenon are also presented. Implications of these studies for the application of the functionalized xenon biosensors in the ordinary and multiplexing capacity are discussed.

Materials and Methods

NMR Experiments. All ^{129}Xe NMR spectra shown were obtained at 83 MHz ($^1\text{H} = 300$ MHz) on a Varian Inova spectrometer. When selective excitation experiments were performed, frequency-selective EBURP1 and IBURP2 pulses⁵⁴ were generated using the PBox program (Varian Instruments). Both selective pulses are designed to excite a bandwidth of 1.8 kHz centered at 10.25 kHz upfield of the frequency of xenon in water, corresponding to a ~ 21.8 ppm excitation window centered about the NMR frequency of xenon bound to water-soluble cryptophanes. Natural-abundance xenon (Isotec or Spectra Gases) was laser-polarized using a commercial polarizer (Amersham Health, Durham, NC) and was introduced to the sample using previously described methods,⁴² with polarizations of 1–5%. To remove molecular oxygen, samples were degassed via several freeze–pump–thaw cycles prior to the introduction of xenon. Experiments involving water-soluble cryptophanes were carried out at 298 K in D_2O . The spectrum of xenon in allyl-functionalized cryptophane (Figure 3a) was obtained at 213 K in a 25% toluene/75% tetrachloroethane solvent mixture. All chemical shifts were referenced by assigning the xenon in D_2O resonance to 195 ppm except for spectra of Figures 3a and 4b–e. The spectrum of Figure 3a was referenced to the shift of xenon gas when extrapolated to 0 atm pressure. The spectra of Figure 4b–e were referenced to the spectrum of Figure 4a. Acquisition time was 1 s with a spectral width of 60 kHz except for exchange-rate measurement data in which the acquisition time was used as the mixing time. Fourier transformed spectra were processed with zero filling and Gaussian line-broadening values of 2 Hz in Figure 3b and c; <10 Hz in Figure 5; 10 Hz in Figures 4, 7, 8; and 20 Hz for intensities integrated in Figure 6. 90° pulses were used for acquiring spectra unless otherwise noted. Exchange-signal averaging was used for the spectra shown in Figure 4c–e ($n = 10$) and also for Figure 6 ($n \geq 3$). Specific pulse sequences for exchange measurement and exchange-signal averaging techniques are presented in the corresponding figures. For both the exchange-signal averaging and the indirect-assay experiments, τ_{mix} was at least 150 ms. Concentrations of particular biosensor samples are noted where relevant and were determined before addition of protein by UV–vis spectrophotometry using a molar absorptivity for water-soluble cryptophanes ($\epsilon_{287} = 8000 \text{ M}^{-1}$), as determined by the dry weight method. The molar

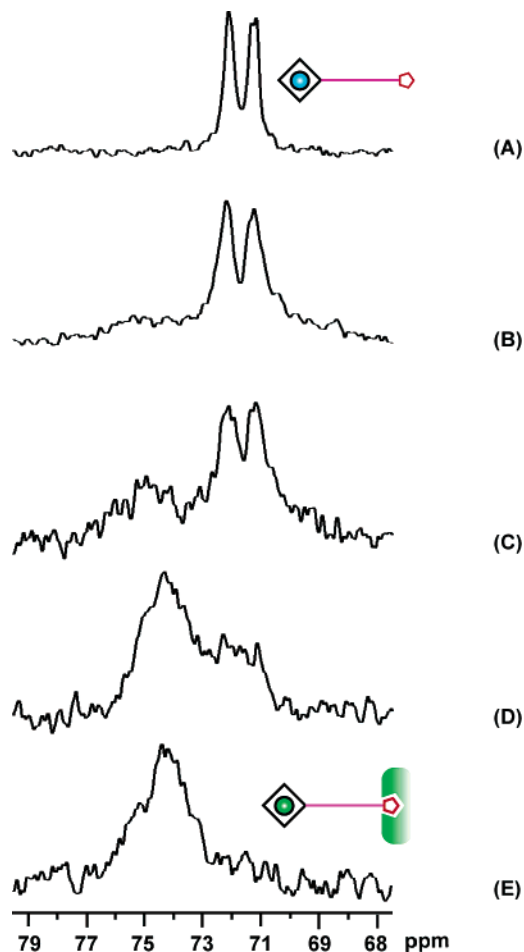


Figure 4. Detection of biotin–avidin binding with xenon NMR. The ^{129}Xe NMR spectra of the functionalized xenon biosensor at various titration points, (A) 0% (300 μM biosensor, 0 μM avidin); (B) 10% (1800 μM , 170 μM); (C) 20% (1800 μM , 350 μM); (D) 60% (300 μM with 180 μM); and (E) 120% (300 μM , 360 μM). These spectra show a new resonance and marked broadening in response to the increasing amounts of avidin. Spectra in (C), (D), and (E) were exchange signal averaged as described in the NMR experimental section.

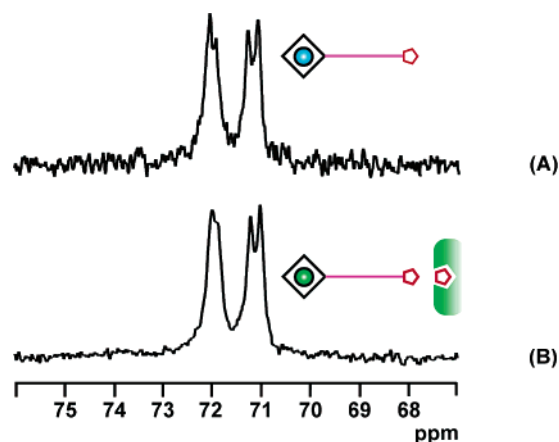


Figure 5. Effect of inhibiting the xenon biosensor binding to avidin. (A) ^{129}Xe spectrum from a solution of the biosensor alone (300 μM); and (B) after addition of approximately 0.5 equiv of avidin (180 μM) that was pre-equilibrated with a 5-fold excess of biotin. These spectra show that the induced shift in Figure 4 is from the specific binding of the biotinylated cage to avidin.

absorptivity for cryptophane in aqueous solution was found to be different than that previously used for cryptophane in organic solution.⁵¹

(54) Geen, H.; Freeman, R. *J. Magn. Reson.* **1991**, *93*, 93–141.

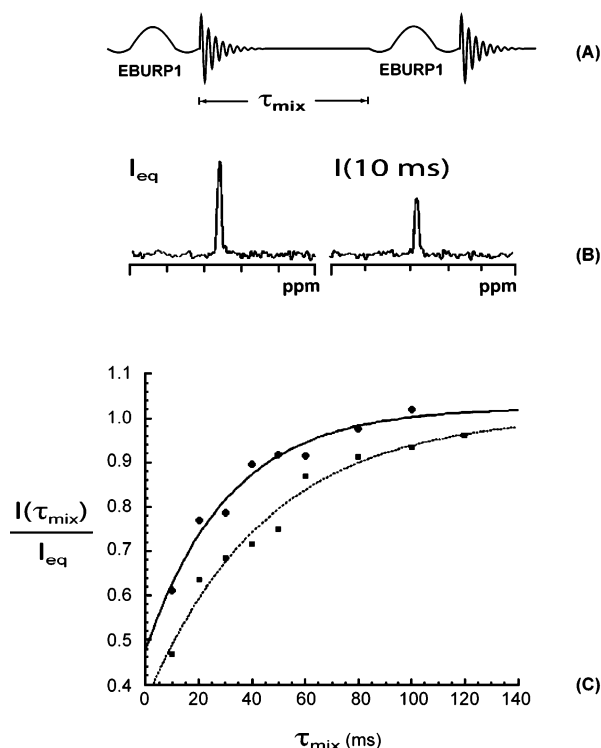


Figure 6. Comparison of xenon exchange with the biosensor cage when biosensor molecule is free (●) and bound (■) to avidin. (A) The pulse sequence for the measurement of the laser-polarized xenon exchange. The first pulse probes the magnetization of the functionalized xenon and selectively saturates the resonance. After time τ_{mix} , the recovery of magnetization through exchange is probed by a second pulse of the same duration. (B) One pair of spectra showing magnetization recovery of biosensor encapsulated xenon at ~ 71.5 ppm after a mixing time of 10 ms. (C) Magnetization recovery curves for 300 μM biosensor/360 μM avidin solution (■) and 300 μM biosensor/360 μM biotin-saturated avidin solution (●) are shown with fitted exponential recovery curves. The nonzero intercept of the curves reflects that each pair of pulses was not set to exactly 90° .

Synthesis. As shown in Figure 2, the water-soluble xenon biosensor (1) was synthesized by attaching a maleimide-activated biotin linker to a peptide-functionalized cryptophane-A cage (2). Cryptophane-A was made water-soluble by attaching the peptide to the cryptophane-acetic acid cage (3), which was prepared using a template method based on that previously reported by Collet and co-workers.^{55–57} A complete description of the synthetic approach and details is included in the Supporting Information.

Results and Discussion

Biosensor Molecule Diastereomers Detected by Functionalized Xenon. Cryptophane-A is chiral,⁵⁵ and xenon dissolved in a racemic mixture of the cage enantiomers gives rise to a single resonance.³¹ Similarly, the xenon spectrum for a racemic mixture of the allyl-substituted cryptophane-A cage enantiomers shows only one resonance upfield from the solvent peak (Figure 3a). The first pair of diastereoisomers is formed by the introduction of chiral L-amino acids Cys, Lys, and Arg. The corresponding xenon spectrum (Figure 3b) of this mixture has two lines separated by 0.15 ppm, attributed to the RL and LL cage-peptide coupled biosensor intermediates. When the peptide-derivatized cage is linked to the biotin linker, a new racemic chiral center is formed at the connection involving the Cys

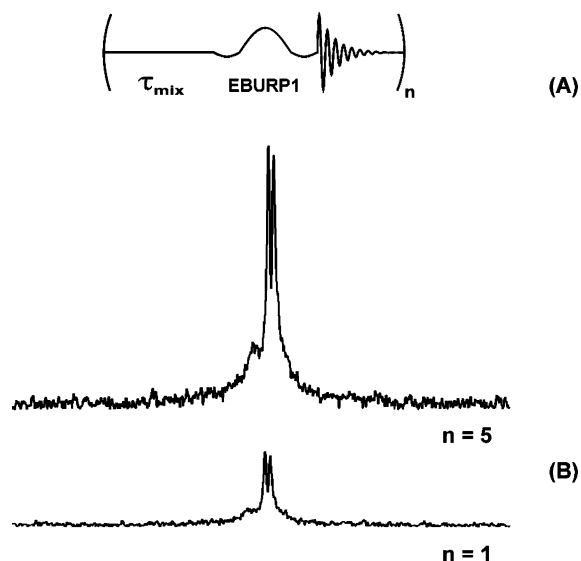


Figure 7. (A) A selective pulse centered about functionalized xenon resonances is used to signal average functionalized xenon peaks. Between selective saturations, the mixing time τ_{mix} allows for the replenishment of functionalized xenon signal by exchanging saturated spins with the polarized xenon dissolved in the surrounding solution. (B) Two spectra of the functionalized xenon peaks comparing one and five scans.

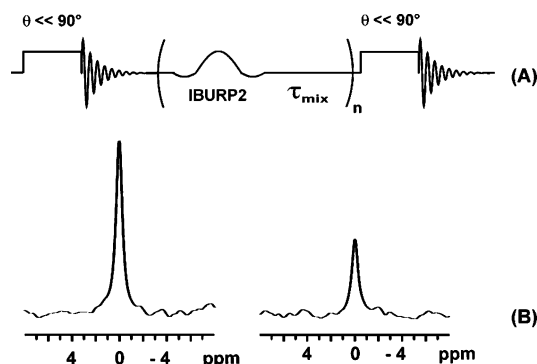


Figure 8. Indirect assay for peptide-derivatized cryptophane-A cage. (A) A selective inversion pulse centered about the functionalized xenon resonances is used to report the presence of functionalized xenon via a decrease in the xenon solution peak. Between selective inversions, the mixing time, τ_{mix} , allows for the depletion of free-xenon signal by exchanging the negatively polarized spins from the cage with the positively polarized xenon that is dissolved in the surrounding solution. (B) A spectrum of the xenon solution peak after the first broadband pulse (left) and a spectrum of the xenon solution peak after five selective inversion pulses ($n = 5$) and the second broadband pulse (right). The solution contained 1.5 mM peptide-derivatized cryptophane-A cage.

residue and the prochiral maleimide (marked with an arrow in Figure 3c). As a result, the cage-peptide-maleimide product is now a mixture of chiral combinations RLR, RLL, LLR, LLL; correspondingly, the spectrum of xenon in the conjugate(s) contains four distinct peaks. The fact that the biotin ligand itself is chiral does not affect the number of peaks predicted because the biotin is enantiomerically pure.

We attribute the four functionalized xenon peaks to distinct xenon chemical shifts arising from the diastereomers of the biosensor molecule. The direct correlation between the number of observed peaks and the number of diastereomers is apparent from Figure 3b,c. The identity of diastereomers has not yet been directly verified, and further experimental studies are needed to better characterize the connection between the chirality of biosensor molecule components and the xenon chemical shift.

(55) Collet, A. *Tetrahedron* **1987**, *43*, 5725–5759.

(56) Brotin, T.; Devic, T.; Lesage, A.; Emsley, L.; Collet, A. *Chem.-Eur. J.* **2001**, *7*, 1561–1573.

Previous studies have provided insight into the chiral nature of the interaction between the xenon chemical shift and the cryptophane-A cage. In the presence of a chiral shift agent, two resonances were observed for xenon encapsulated in a racemic mixture of cryptophane-A.^{58,59} Experimental studies using xenon to report the interconversion of two diastereomers, α - and β -glucose,⁶⁰ as well as theoretical studies using model helices have helped to clarify the interaction of xenon with diastereomers.^{61–64}

Previous experimental studies, which are now being understood with theoretical models by Sears and Jameson,⁶⁵ have shown that direct changes to the basic structure of the cryptophane-A cage perturb the chemical shift of the cryptophane-encapsulated xenon. For example, a 30 ppm change in chemical shift was noted when the length of the bridges between the cyclotrimerethylene caps of cryptophane-A was increased by one methylene group,⁵¹ and even deuteration of a single methoxy group on a cryptophane-A cage has been shown to produce a noticeable shift (~ 0.1 ppm).⁶⁶ In this work, we show that significant xenon chemical shift differences also result from derivatizations of cryptophane-A that are not local to the encapsulated xenon. The presence of chiral centers attached to the outside of the cage cause changes of up to ~ 1 ppm in the xenon chemical shift. The sensitivity of xenon to indirect changes in cage structure or environment is important for distinguishing bound and free ligand in addition to offering greater potential for multiplexing the xenon biosensor. By combining different chemical changes in and around the cryptophane, it will be possible to tune the chemical shift of the xenon in the cage, making it possible to follow binding events of different ligand–cage combinations in parallel.⁵¹

Characteristics of Protein-Bound Functionalized Xenon Spectrum. Titration of Biotinylated Functionalized Xenon Biosensor with Avidin Protein. We previously showed that the chemical shift of the biotinylated cryptophane-A biosensor is sensitive to the presence of avidin.⁵¹ We have now extended the experiments to a complete titration of the free biosensor with avidin (Figure 4), showing that increasing amounts of avidin lead to corresponding changes in the xenon spectrum. Biosensor-avidin solutions used for Figure 4a–e have amounts of avidin monomer that are 0%, 10%, 20%, 60%, and 120% of the total biosensor concentration, respectively (see figure caption for concentration values). The addition of avidin to free biosensor leads to the appearance of a broad, downfield resonance accompanied by a decrease in the intensity of the free biosensor resonances (Figure 4b). The spectral changes continue in this manner with increasing amounts of avidin (Figure 4c,d). The addition of a full equivalent of avidin results

in a single peak about 3 ppm downfield (Figure 4e). The appearance of a single, broadened peak for protein-bound biosensor indicates that functionalized xenon resonances undergo a significant increase in line width when compared to those of the free biosensor.

Verification of Correspondence between Spectral Changes and Binding Event. When the biotinylated xenon biosensor (300 μM) is added to avidin (180 μM) that had been pre-equilibrated with a 5-fold excess of normal biotin, the xenon spectrum is unchanged as compared to that of the same concentration of biosensor alone (Figure 5). This control experiment demonstrates that the appearance of the downfield peak arises from specific binding of the biotin portion of the functionalized xenon biosensor to avidin, rather than from nonspecific interactions with the protein. This also makes clear that specific binding of the biosensor to avidin is responsible for broadening of the functionalized xenon resonances. The broad lines from the biosensor–protein complex have contributions from homogeneous broadening and the distribution of diastereomeric shifts.

Exchange Measurements. The biosensor–protein binding event may decrease the lifetime of xenon in the cage, thereby making exchange line-broadening more efficient. To determine whether this was the case, the exchange rates were measured for both free and protein-bound biosensor.

The exchange of xenon between cage and solution was determined by measuring the recovery of selectively saturated functionalized xenon signal. The pulse sequence used is shown in Figure 6a, in which all pulses are $\sim 90^\circ$ chemical-shift-selective pulses centered on the resonance frequency of functionalized xenon as described in the experimental section. The initial observation of the z-magnetization of the functionalized xenon is followed by an exchange delay, τ_{mix} , followed by another observation of the z-magnetization. The measurement of the signal intensity following the first pulse allows for the normalization of exchange-recovered intensity observed by the second pulse (Figure 6b). Without exchange, recovery of magnetization would be negligible as the equilibrium magnetization is small relative to the initial magnetization achieved with laser-polarization. The growth of magnetization during τ_{mix} occurs only through exchange with polarized xenon atoms in the solvent, allowing the rate to be determined via curve-fitting to a pseudo-first-order exchange mechanism,⁶⁷ as shown in Figure 6c. This method presumes that a single saturation of the functionalized xenon resonance does not significantly change the polarization of the xenon free in solution and that no significant spin–lattice relaxation of free xenon occurs between the first and second saturations. These are reasonable assumptions as free xenon is present in greater than 10-fold excess, and the spin–lattice relaxation time of free xenon in these solutions is on the order of hundreds of seconds, as measured by probing the longitudinal magnetization of the free xenon using tipping angles of $\sim 3^\circ$ at regular intervals (data not shown).

Figure 6c shows the data points and fits for exchange measurements of the free and avidin-bound functionalized xenon solutions. The exchange lifetimes determined are 30 ± 8 ms for free functionalized xenon and 45 ± 11 ms for protein-bound functionalized xenon. The exchange lifetime for free functionalized xenon is consistent with the line width of ~ 15 Hz

- (57) Kilenyi, S. N.; Mahaux, J. M.; Vandurme, E. *J. Org. Chem.* **1991**, *56*, 2591–2594.
(58) Bartik, K.; El Haouaj, M.; Luhmer, M.; Collet, A.; Reisse, J. *ChemPhysChem* **2000**, *1*, 221–224.
(59) Bartik, K.; Luhmer, M.; Collet, A.; Reisse, J. *Chirality* **2001**, *13*, 2–6.
(60) Locci, E.; Reisse, J.; Bartik, K. *ChemPhysChem* **2003**, *3*, 305–308.
(61) Sears, D. N.; Jameson, C. J.; Harris, R. A. *J. Chem. Phys.* **2003**, *119*, 2685–2690.
(62) Sears, D. N.; Jameson, C. J.; Harris, R. A. *J. Chem. Phys.* **2003**, *119*, 2691–2693.
(63) Sears, D. N.; Jameson, C. J.; Harris, R. A. *J. Chem. Phys.* **2003**, *119*, 2694–2701.
(64) Sears, D. N.; Jameson, C. J.; Harris, R. A. *J. Chem. Phys.* **2004**, *120*, 3277–3283.
(65) Sears, D. N.; Jameson, C. J. *J. Chem. Phys.* **2003**, *119*, 12231–12244.
(66) Brotin, T.; Lesage, A.; Emsley, L.; Collet, A. *J. Am. Chem. Soc.* **2000**, *122*, 1171–1174.

- (67) McConnell, H. M. *J. Chem. Phys.* **1958**, *28*, 430–431.

observed in corresponding spectra, suggesting that the exchange process is the dominant mechanism for line-broadening in the absence of protein. The similarity in exchange rate values for free and protein-bound biosensor indicates that increased broadening upon binding is not caused by an increase in the exchange rate of xenon between the cage and solvent. Thus, the broadening observed upon binding is most likely caused by the increase in rotational correlation time of the cage that dictates transverse (T_2) relaxation time of xenon inside the cage. Binding of the biosensor molecule to a comparatively large protein should lengthen the correlation time of the cage considerably, leading to an increased efficiency of relaxation through dipole–dipole coupling and chemical shift anisotropy. Due to the high spin-polarization of ^{129}Xe , significant xenon-to-proton cross-relaxation has been observed to protonated liquids,⁶⁸ proteins,^{69,70} and also cryptophane cage protons.^{71,72} Studies at different magnetic fields as well as studies with deuterated cages should help distinguish contributions from the two mechanisms.

Exchange rates comparable to those of xenon in the biosensor have been measured previously for xenon–cryptophane complexes in organic solutions at very low temperatures.⁶⁶ In organic solvents at room temperature, cryptophane-A-bound xenon shows exchanged-broadened line widths of hundreds of hertz,³¹ suggesting exchange rates more than an order of magnitude higher than those measured here. The slower exchange reflected in the narrower lines of the water-soluble xenon–cryptophane-A complex presented here suggests a higher binding constant of xenon in water than organic solvents, consistent with a larger hydrophobic contribution to the binding.

Methods for Enhancing Biosensor Sensitivity. In conventional-NMR signal averaging, individual scans are comprised of excitation, followed by acquisition and signal-recovery periods in which the magnetization is allowed to return toward thermal equilibrium. Experiments involving laser-polarized xenon are not amenable to this type of signal averaging because the large initial magnetization is nonequilibrium. Following the first acquisition, the xenon would relax back to its small, equilibrium polarization, and subsequent scans would add negligible signal to the initial contribution of hyperpolarized xenon signal. Reestablishing the polarization requires adding more laser-polarized xenon to the sample, a substantial cost in experiment time.

Modified pulse sequences are often employed in laser-polarized xenon NMR spectroscopy and imaging to maximize use of the xenon magnetization.^{73,74} The exchange properties of the biosensor system presented here allow for the implementation of novel signal enhancement techniques using modified pulse sequences. The application of selective pulses is accomplished easily due to the large separation (~ 120 ppm) between xenon resonances in solution and in cages. The slow-

exchange characteristic allows for the selective detection of free and functionalized xenon resonances by use of selective pulses to manipulate the two sets of spins independently. The exchange is relatively rapid in comparison to the longitudinal relaxation time of xenon, allowing for replenishment of biosensor-bound xenon polarization after saturation with little loss of signal between identical acquisitions. In the following sections, we exploit these convenient exchange properties to increase biosensor sensitivity.

Exchange-Signal Averaging. The identification of a protein binding event by observation of a shift and broadening in the spectrum only requires the spectral region including the caged-xenon resonance and not that from xenon in the solvent. The cryptophane-bound xenon can be selectively excited using chemical-shift selective pulses. The polarization of xenon in the solvent is left to serve as a magnetization reservoir from which functionalized xenon magnetization is replenished following an appropriate mixing time, τ_{mix} . Repeat acquisitions of functionalized xenon spectra are added to result in a higher signal-to-noise spectrum. However, the magnetization of the xenon in solvent is a finite reservoir, limiting the number of spectra contributing a signal-to-noise enhancement to the average. Estimates of the bulk xenon T_1 value as well as the concentrations of both biosensor molecule and dissolved xenon allow an accurate calculation of how much averaging is beneficial. Figure 7a shows the pulse sequence used to accomplish exchange-signal averaging. An example of signal averaging is shown in Figure 7b for five scans ($n = 5$). The signal-to-noise ratio has increased approximately by 2-fold relative to the single scan spectrum because this number of scans has not significantly depleted the polarization reservoir in the solvent and T_1 relaxation is negligible during the course of the experiment.

Signal averaging can afford a large sensitivity increase for xenon biosensor detection of dilute analytes, where the concentration of the analyte is much less than that of xenon in water. These averages can be repeated on the time scale of the magnetization exchange, tens of milliseconds, in contrast to the required relaxation delay for conventional signal averaging. Furthermore, the very large signal of xenon in water is not observed, eliminating the problem of dynamic range introduced by the coexistence of two signals of significantly different intensities, similar to that of proton NMR in the presence of water.

Indirect Assay for the Biosensor Event by Xenon Exchange. In the simplest case, a xenon biosensor assay only requires relating a measurement of magnetization intensity to a quantity of protein-bound biosensor. This does not necessitate the acquisition of a functionalized xenon spectrum. Here, we introduce a method, Figure 8a, that measures changes in the magnetization of free xenon in solution that are proportional to the amount of xenon biosensor. This method utilizes exchange of xenon between the functionalized and solvent environments to indirectly assay for the presence of xenon biosensor. Following a probe pulse (tip angle of $\sim 10^\circ$) to measure the initial magnetization of xenon in solution, multiple, selective inversions of functionalized xenon magnetization are carried out to measurably reduce the magnetization of free xenon. An appropriate repetition rate of $\sim 5 \times \tau_{\text{ex}}$ between inversion pulses allows the resulting, decreased magnetization of free xenon to

(68) Navon, G.; Song, Y. Q.; Room, T.; Appelt, S.; Taylor, R. E.; Pines, A. *Science* **1996**, *271*, 1848–1851.

(69) Berthault, P.; Landon, C.; Vovelle, F.; Desvaux, H. *C. R. Acad. Sci. IV-Phys.* **2001**, *2*, 327–332.

(70) Landon, C.; Berthault, P.; Vovelle, F.; Desvaux, H. *Protein Sci.* **2001**, *10*, 762–770.

(71) Luhmer, M.; Goodson, B. M.; Song, Y. Q.; Laws, D. D.; Kaiser, L.; Cyriac, M. C.; Pines, A. *J. Am. Chem. Soc.* **1999**, *121*, 3502–3512.

(72) Desvaux, H.; Huber, J. G.; Brotin, T.; Dutasta, J. P.; Berthault, P. *Chemphyschem* **2003**, *4*, 384–387.

(73) Patyal, B. R.; Gao, J. H.; Williams, R. F.; Roby, J.; Saam, B.; Rockwell, B. A.; Thomas, R. J.; Stolarski, D. J.; Fox, P. T. *J. Magn. Reson.* **1997**, *126*, 58–65.

(74) Ruppert, K.; Brookeman, J. R.; Hagspiel, K. D.; Mugler, J. P. *Magn. Reson. Med.* **2000**, *44*, 349–357.

directly reflect the amount of xenon biosensor, as measured by another probe pulse.

Figure 8b shows the application of the indirect assay ($n = 5$) to a solution containing 1.5 mM of peptide-derivatized cryptophane-A cage (**2**, Figure 2). The decrease in the integrated intensity of the solution peak by 60% reflects the presence of the cryptophane-bound xenon. Contributions to reduction in signal intensity from other factors including the initial tip pulse, T_1 relaxation, and shaped pulse error were investigated. This was done by repeating the indirect assay with an off-resonance inversion pulse. The shaped pulse, which is normally centered about the functionalized xenon spins, is placed at an equal but opposite offset from the solution resonance. By mirroring the position of the shaped pulse, inversion of the biosensor magnetization is eliminated while maintaining an identical residual excitation of free xenon in both experiments. In addition, the delay between probe pulses ($n = 5$; $\tau_{\text{mix}} = 150$ ms) is unchanged in the off-resonance experiment allowing for equal T_1 reduction in free xenon magnetization as compared to that of an on-resonance indirect assay. We found a 10% reduction in magnetization intensity after applying the off-resonance indirect assay pulse sequence, indicating the full reduction of signal intensity is associated with the presence of cryptophane-bound xenon.

The indirect assay for the xenon biosensor has sensitivity advantages over signal averaging. Its signal-to-noise ratio scales directly with the number of scans because the signal is acquired after the biosensor magnetization has accumulated. Unlike the functionalized xenon signal, the observed solution-xenon signal not only scales with increasing laser-polarization, but also scales directly with the concentration of dissolved xenon. Hence, the limit of detection in terms of biosensor concentration is reduced. A full description of the application of this technique to quantitatively report and distinguish free and bound biosensor will be presented elsewhere.

Conclusions

The magnetic resonance properties of encapsulated xenon tethered to biotin, both free and bound to avidin, have been characterized. Diastereomeric combinations of cage and biotin linker explain the presence of multiple lines observed in the functionalized xenon spectra. This suggests that the sensitivity of xenon to subtle changes in cage structure can be exploited to create sets of sensors that can be detected in parallel, thereby allowing for multiplexing at the chemical level. A full titration of the xenon biosensor with avidin is presented, showing a marked broadening of the xenon biosensor upon avidin binding. An increase in the xenon exchange rate was ruled out as a source of this broadening because the rate of xenon transfer is not significantly altered when the cage derivative binds to the protein. This rate is sufficiently slow that it does not contribute significantly to the line width of the protein-bound biosensor resonance. The broadening of the protein-bound functionalized xenon resonance results from an increase in the correlation time of the higher molecular weight complex through dipole–dipole and perhaps chemical shift anisotropy mechanisms. Asymmetrically hydroxyl-derivatized cryptophane-A cages termed cryptophanols, which were developed independently by Dutasta and co-workers,⁷⁵ may also be used for the preparation of biosensor molecules. Dutasta and co-workers have also shown that

cryptophanol-A cages can be partially deuterated,⁷⁶ and use of these unique constructs in biosensor molecules should allow for experiments that distinguish the dipolar and CSA relaxation contributions to line-broadening of biosensor resonances. Particularly, reduction in the dipolar coupling by deuteration should improve the line width and sensitivity of biosensor experiments. Another approach that may reduce relaxation efficiency involves changing the length of the tether between the cage and biotin. A longer linker might allow more independent motion of the cryptophane-A cage, decreasing its correlation time and slowing xenon relaxation. In using this approach, we must consider the possible reduction in the binding-induced shift response of the biosensor, if the shift mechanism depends on contact between the cage and protein. Recent theoretical studies by Sears and Jameson⁶⁵ have accurately modeled the response of xenon's chemical shift to a given cage structure by the careful averaging of different cage configurations sampled by the encapsulated xenon during an NMR experiment; consequently, it is possible that the chemical shift change of a long-linker biosensor arises from subtle distortions of the cage induced by changes in its vibrational and rotational motions, and this shift mechanism could still be effective even with a longer linker.

Signal enhancement using the exchange properties of the laser-polarized xenon biosensor was demonstrated to improve detection sensitivity. The techniques presented here are applicable to any system which binds xenon such that the exchange rate is slow on the chemical shift time scale, but fast on the spin–lattice relaxation time scale; a number of cage molecules in the solid state and in solution show affinity and exchange properties for xenon.^{28–30,32,33} Exchange-signal enhancement of the xenon biosensor may extend its application to environments where analyte concentration is expected to be very low, such as for in vivo spectroscopy and imaging.⁷⁷ Moreover, it offers the possibility for even higher sensitivity remote detection.

Acknowledgment. We thank Robert A. Harris (for his indispensable role in the discovery of xenon detected diastereomer molecules), as well as Cynthia J. Jameson and Devin Sears for fruitful discussions regarding the diastereomeric chemical shifts of xenon. We thank Nycomed Amersham for sharing their knowledge of batch polarization techniques. M.M.S. and S.M.R. acknowledge the National Science Foundation, E.J.R. acknowledges Lucent Technologies/Bell Laboratories and UC Berkeley for predoctoral fellowships, and N.W. acknowledges the National Institutes of Health for his postdoctoral fellowship. This work was supported by the Director, Office of Science, Office of Basic Energy Sciences, Materials Sciences Division and Physical Biosciences Division of the U.S. Department of Energy under Contract No. DE-AC03-76SF00098.

Supporting Information Available: Synthetic strategy and synthetic details, figure showing the retrosynthesis of derivatized cryptophane, and schemes showing the syntheses of **8**, **16**, and biotin-derivatized cryptophane. This material is available free of charge via the Internet at <http://pubs.acs.org>.

JA0483037

- (75) Darzac, M.; Brotin, T.; Bouchu, D.; Dutasta, J. P. *Chem. Commun.* **2002**, 48–49.
(76) Darzac, M.; Brotin, T.; Rousset-Arzel, L.; Bouchu, D.; Dutasta, J. P. *New J. Chem.* **2004**, 502–512.
(77) Lowery, T. J.; Rubin, S. M.; Ruiz, E. J.; Spence, M. M.; Winssinger, N.; Schultz, P. G.; Pines, A.; Wemmer, D. E. *Magn. Reson. Imaging* **2003**, *21*, 1235–1239.