

Enzyme-Amplified Array Sensing of Proteins in Solution and in Biofluids

Oscar R. Miranda,[†] Hung-Ting Chen,[†] Chang-Cheng You,[†] David E. Mortenson,[†] Xiao-Chao Yang,[§] Uwe H. F. Bunz,[‡] and Vincent M. Rotello*[†]

Department of Chemistry, University of Massachusetts, 710 North Pleasant Street, Amherst, Massachusetts 01003, School of Chemistry and Biochemistry, Georgia Institute of Technology, 901 Atlantic Drive, Atlanta, Georgia 30332, and College of Bioengineering and Microsystem Research Center, Chongqing University, Chongqing 400044, People's Republic of China

Received January 25, 2010; E-mail: rotello@chem.umass.edu

Abstract: We have developed an enzyme–nanoparticle sensor array where the sensitivity is amplified through enzymatic catalysis. In this approach cationic gold nanoparticles are electrostatically bound to an enzyme (β -galactosidase, β -Gal), inhibiting enzyme activity. Analyte proteins release the β -Gal, restoring activity and providing an amplified readout of the binding event. Using this strategy we have been able to identify proteins in buffer at a concentration of 1 nM, substantially lower than current strategies for array-based protein sensing. Moreover, we have obtained identical sensitivity in studies where the proteins are spiked into the complex protein matrix provided by desalted human urine ($\sim 1.5 \mu\text{M}$ total protein; spiked protein concentrations were 0.067% of the overall protein concentration), demonstrating the potential of the method for diagnostic applications.

Introduction

Irregular protein concentration levels in biofluids, e.g., serum, urine, and saliva, provide essential information for the early diagnosis of many pathological conditions such as hypoalbuminemia,¹ cancers,² Alzheimer's disease,³ prostatitis,⁴ HIV,⁵ and other disease states.⁶ The development of strategies for monitoring protein levels remains a major issue in medical diagnostics, pathogen detection, and proteomics.⁷ Substantial efforts have been devoted to develop precise and efficient

methods for protein sensing,⁸ including enzyme-labeled immunoassays,⁹ electrophoresis methods,¹⁰ and analytical techniques.¹¹

The “chemical nose/tongue” approach¹² presents a potential alternative to specific recognition and separations techniques. In this approach, a sensor array is generated to provide differential interaction with analytes via *selective* receptors,

[†] University of Massachusetts.

[‡] Georgia Institute of Technology.

[§] Chongqing University.

- (1) (a) Abdelhafiz, A. H.; Myint, M. P.; Tayek, J. A.; Wheeldon, N. M. *Clin. Ther.* **2009**, *21*, 1534. (b) Galic, G.; Tomic, M.; Galesic, K.; Kvesic, A.; Soljic, M.; Mozetic, V.; Loncar, Z.; Maricic, A.; Martinovic, Z. *Coll. Antropol.* **2009**, *33*, 559. (c) Zismam, D. A.; Kawut, S. M.; Lederer, D. J.; Belperio, J. A.; Lynch, J. P.; Schwarz, M. I.; Tayek, J. A.; Reuben, D. B.; Karlamangla, A. S. *Chest* **2009**, *135*, 929. (d) Abdelhafiz, A. H.; Wheeldon, N. M. *Clin. Ther.* **2004**, *26*, 1470. (e) Abdelhafiz, A. H.; Wheeldon, N. M. *Am. J. Geriatr. Pharmacother.* **2008**, *6*, 1.
- (2) (a) Hogdall, E. V. S.; Christensen, L.; Kjaer, S. K.; Blaakaer, J.; Kjaerbye-Thygesen, A.; Gayther, S.; Jacobs, I. J.; Hogdall, C. K. *Gynecol. Oncol.* **2007**, *104*, 508. (b) Daniels, M. J.; Wang, Y.; Lee, M.-Y.; Venkitaraman, A. R. *Science* **2004**, *306*, 876. (c) Ross, J. S.; Fletcher, J. A. *Stem Cells* **1998**, *16*, 413.
- (3) (a) Couderc, R. *Ann. Biol. Clin.* **2000**, *58*, 581. (b) Yaffe, K.; Barrett-Connor, E.; Lin, F.; Grady, D. *Arch. Neurol.* **2002**, *59*, 378. (c) Saunders, A. M.; Strittmatter, W. J.; Schmechel, D.; George-Hyslop, P. H.; Pericak-Vance, M. A.; Joo, S. H.; Rossi, B. L.; Gusella, J. F.; Crapper-MacLachlan, D. R.; Alberts, M. J.; Hulette, C.; Crain, B.; Goldgaber, D.; Roses, A. D. *Neurology* **1993**, *43*, 1467. (d) Padmanabhan, J.; Levy, M.; Dickson, D. W.; Potter, H. *Brain* **2006**, *129*, 3020. (e) Hampel, H.; Burger, K.; Teipel, S. J.; Bokde, A. L.; Zetterberg, H.; Blennow, K. *Alzheimer's Dementia* **2008**, *4*, 38. (f) Andreasson, U.; Portelius, E.; Andersson, M. E.; Blennow, K.; Zetterberg, H. *Biomarkers Med.* **2007**, *1*, 59.

- (4) (a) Tricoli, J. V.; Schoenfeldt, M.; Conley, B. *Clin. Cancer Res.* **2004**, *10*, 3943. (b) Bai, V. U.; Kaseb, A.; Tejwani, S.; Divine, G. W.; Barrack, E. R.; Menon, M.; Pardee, A. B.; Reddy, G. P. V. *Proc. Natl. Acad. Sci.* **2007**, *104*, 2343. (c) Gutman, A. B.; Gutman, E. B. *J. Clin. Invest.* **1938**, *17*, 473. (d) Brawer, M. K.; Chetner, M. P.; Beatie, J.; Buchner, D. M.; Vessella, R. L.; Lange, P. H. *J. Urology* **1992**, *147*, 841. (e) Deftos, L. J.; Abrahamsson, P. A. *Urology* **1998**, *51*, 141. (f) Pisitkun, T.; Johnstone, R.; Knepper, M. A. *Mol. Cell. Proteomics* **2006**, *5*, 1760.

- (5) (a) Payne, B. A. I.; Price, D. A.; Schmid, M. L.; Ong, E.; Snow, M. H. *J. Infect.* **2007**, *54*, e195. (b) Nielsen, S. L.; Andersen, P. L.; Koch, C.; Jensenius, J. C.; Thiel, S. *Clin. Exp. Immunol.* **1995**, *100*, 219. (c) Cantry, O.; Moja, P.; Quesnel, A.; Pozzetto, B.; Lucht, F. R.; Genin, C. *Clin. Exp. Immunol.* **1997**, *109*, 47.
- (6) (a) Hardy, J.; Selkoe, D. J. *Science* **2002**, *297*, 353. (b) Pulido, R.; van Huijsduijn, R. H. *FEBS J.* **2008**, *275*, 848. (c) Masson, J.-F.; Battaglia, T. M.; Khairallah, P.; Beaudoin, S.; Booksh, K. S. *Anal. Chem.* **2007**, *79*, 612.
- (7) Kodadek, T. *Chem. Biol.* **2001**, *8*, 105.
- (8) (a) Soukka, T.; Paukkunen, J.; Harma, H.; Lonnberg, S.; Lindroos, H.; Lovgren, T. *Clin. Chem.* **2001**, *47*, 1269. (b) Acharya, G.; Chang, C.-L.; Doorneweerd, D. D.; Vlashi, E.; Henne, W. A.; Hartmann, L. C.; Low, P. S.; Savran, C. A. *J. Am. Chem. Soc.* **2007**, *129*, 15824. (c) Muller, U. R. *Mol. Biosyst.* **2006**, *2*, 470.
- (9) (a) Engvall, E.; Perlmann, P. *J. Immunol.* **1972**, *109*, 129. (b) Schuur, A. H. W. M.; Van Weemen, B. K. *J. Immunoassay* **1980**, *1*, 229. (c) Haab, B. B. *Curr. Opin. Biotechnol.* **2006**, *17*, 415.
- (10) McPherson, R. A.; Pincus, M. R. *Henry's Clinical Diagnosis and Management by Laboratory Methods*; Saunders-Elsevier, 2007; Chapter 19.
- (11) (a) Li, J. N.; Zhang, Z.; Rosenzweig, J.; Wang, Y. Y.; Chan, D. W. *Clin. Chem.* **2002**, *48*, 1296. (b) Baggerly, K. A.; Morris, J. S.; Coombes, K. R. *Bioinformatics* **2004**, *20*, 777.

generating a stimulus response pattern that can be statistically analyzed and used for the identification of individual target analytes^{13,14} and also analysis of complex mixtures.¹⁵ Over the past few years, this technology has been successfully applied for protein detection using array-based approaches, including porphyrins,¹⁶ oligopeptide-functionalized resins,¹⁷ and polymers.¹⁸ In a real-world example, a single functional conjugated polymer, poly(thiophene), has been successfully applied as a food freshness sensor to detect biogenic amines in fish associated with food poisoning (e.g., histamine) with increasing concentrations from 22.5 μM (2.5 ppm) to 4.5 mM (500 ppm) to build a fish matrix.¹⁹ Recently, we have developed nanoparticle–GFP-based “chemical nose” strategy for protein detection in biofluid that is highly sensitive (500 nM)²⁰ as compared to other reported similar approaches (1–350 μM).^{16,17,18c} We have also developed a sensor array composed of gold nanoparticles and fluorescent polymers that can identify proteins,²¹ bacteria,²² and cancerous cells²³ through a fluorophore-displacement mechanism. This sensor array achieved detection limits of 215 nM for low M_w proteins.

- (12) (a) Goodey, A.; Lavigne, J. J.; Savoy, S. M.; Rodriguez, M. D.; Curey, T.; Tsao, A.; Simmons, G.; Wright, J.; Yoo, S. J.; Sohn, Y.; Ansyn, E. V.; Shear, J. B.; Neikirk, D. P.; McDevitt, J. T. *J. Am. Chem. Soc.* **2001**, *123*, 2559. (b) Albert, K. J.; Lewis, N. S.; Schauer, C. L.; Sotzing, G. A.; Stitzel, S. E.; Vaid, T. P.; Walt, D. R. *Chem. Rev.* **2000**, *100*, 2595.
- (13) (a) Wiskur, S. L.; Floriano, P. N.; Ansyn, E. V.; McDevitt, J. T. *Angew. Chem., Int. Ed.* **2003**, *42*, 2070. (b) Lavigne, J. J.; Savoy, S. M.; Clevenger, M. B.; Ritchie, J. E.; McDoniel, B.; Yoo, S. J.; Ansyn, E. V.; McDevitt, J. T.; Shear, J. B.; Neikirk, D. P. *J. Am. Chem. Soc.* **1998**, *120*, 6429. (c) Curey, T. E.; Goodey, A.; Tsao, A.; Lavigne, J. J.; Sohn, Y.; McDevitt, J. T.; Ansyn, E. V.; Neikirk, D.; Shear, J. B. *Anal. Biochem.* **2001**, *293*, 178. (d) McCleskey, S. C.; Griffin, M. J.; Schneider, S. E.; McDevitt, J. T.; Ansyn, E. V. *J. Am. Chem. Soc.* **2003**, *125*, 1114.
- (14) (a) Folmer-Andersen, J. F.; Kitamura, M.; Ansyn, E. V. *J. Am. Chem. Soc.* **2006**, *128*, 5652. (b) Buryak, A.; Severin, K. A. *J. Am. Chem. Soc.* **2005**, *127*, 3700. (c) Greene, N. T.; Shimizu, K. D. *J. Am. Chem. Soc.* **2005**, *127*, 5695. (d) Wright, A. T.; Ansyn, E. V. *Chem. Soc. Rev.* **2006**, *35*, 14. (e) Lee, J. W.; Lee, J.-S.; Chang, Y.-T. *Angew. Chem., Int. Ed.* **2006**, *45*, 6485. (f) Rakow, N. A.; Suslick, K. S. *Nature* **2000**, *406*, 710.
- (15) (a) Rakow, N. A.; Suslick, K. S. *Nature* **2000**, *406*, 710. (b) Krantz-Rulcker, C.; Stenberg, M.; Winquist, F.; Lundstrom, I. *Anal. Chim. Acta* **2001**, *426*, 217. (c) Lewis, N. S. *Acc. Chem. Res.* **2004**, *37*, 663. (d) Collins, B. E.; Wright, A. T.; Ansyn, E. V. *Top. Curr. Chem.* **2007**, *277*, 181. (e) Buryak, A.; Pozdnoukhov, A.; Severin, K. *Chem. Commun.* **2007**, 2366. (f) Wright, A. T.; Edwards, N. Y.; Ansyn, E. V.; McDevitt, J. T. *Angew. Chem., Int. Ed.* **2007**, *46*, 8212. (g) Stephenson, C. J.; Shimizu, K. D. *Polym. Int.* **2007**, *56*, 482.
- (16) (a) Baldini, L.; Wilson, A. J.; Hong, J.; Hamilton, A. D. *J. Am. Chem. Soc.* **2004**, *126*, 5656. (b) Zhou, H.; Baldini, L.; Hong, J.; Wilson, A. J.; Hamilton, A. D. *J. Am. Chem. Soc.* **2006**, *128*, 2421.
- (17) Wright, A. T.; Griffin, M. J.; Zhong, Z. L.; McCleskey, S. C.; Ansyn, E. V.; McDevitt, J. T. *Angew. Chem., Int. Ed.* **2005**, *44*, 6375.
- (18) (a) Miranda, O. R.; You, C.-C.; Phillips, R.; Kim, I. B.; Ghosh, P. S.; Bunz, U. H. F.; Rotello, V. M. *J. Am. Chem. Soc.* **2007**, *129*, 9856. (b) Sandanaraj, B. S.; Demont, R.; Aathimaniikandan, S. V.; Savariar, E. N.; Thayumanavan, S. *J. Am. Chem. Soc.* **2006**, *128*, 10686. (c) Sandanaraj, S. B.; Demont, R.; Thayumanavan, S. *J. Am. Chem. Soc.* **2007**, *129*, 3506.
- (19) Maynor, M. S.; Nelson, T. L.; O’Sullivan, C.; Lavigne, J. J. *Org. Lett.* **2007**, *9*, 3217.
- (20) De, M.; Rana, S.; Akpinar, H.; Miranda, O. R.; Arivizo, R.; Bunz, U. H. F.; Rotello, V. M. *Nat. Chem.* **2009**, *1*, 461.
- (21) You, C.-C.; Miranda, O. R.; Gider, B.; Ghosh, P. S.; Kim, I. B.; Erdogan, B.; Krovi, S. A.; Bunz, U. H. F.; Rotello, V. M. *Nat. Nanotechnol.* **2007**, *2*, 318.
- (22) Phillips, R. L.; Miranda, O. R.; You, C. C.; Rotello, V. M.; Bunz, U. H. F. *Angew. Chem., Int. Ed.* **2008**, *47*, 2590.
- (23) Bajaj, A.; Miranda, O. R.; Kim, I.-B.; Phillips, R. L.; Jerry, D. J.; Bunz, U. H. F.; Rotello, V. M. *Proc. Natl. Acad. Sci.* **2009**, *106*, 10912.

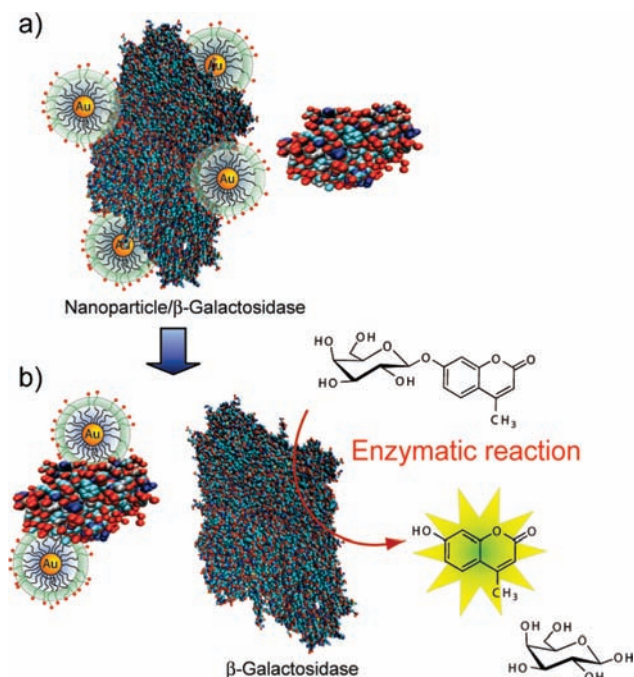


Figure 1. Schematic representation of sensors comprised of β -galactosidase (β -Gal) and cationic AuNPs. In (a) supramolecular adducts of β -Gal and AuNP formed through complementary electrostatic interactions, inhibiting the enzymatic activity of β -galactosidase. As shown in (b) β -galactosidase is displaced from the β -Gal/AuNP complex by protein analytes, restoring the catalytic activity of β -Gal toward the fluorogenic substrate 4-methylumbelliferyl- β -D-galactopyranoside, resulting in an amplified signal for detection.

The increased sensitivity required for many diagnostic uses²⁴ presents a challenging goal for array-based sensors because the detection process generally relies on fluorescence responses that are restricted by the inherent emissivity of the fluorophores used. To overcome this limitation, we have explored the use of enzymes to provide array-based sensors with enhanced sensitivity. In this enzyme-amplified array sensing (EAAS) approach, the sensitivity of the array is amplified through an enzymatic reaction. This approach couples the signal amplification process of ELISA with the versatility of the “chemical nose” approach. We report here the use of this method to sense and identify a range of biomedically relevant proteins at 1 nM in both buffer and desalted human urine.

Our EAAS features three components: (a) β -galactosidase (β -Gal) as the enzyme, (b) 4-methylumbelliferyl- β -D-galactopyranoside (MUG) as a fluorogenic substrate to provide “turn on” sensing, and (c) gold nanoparticles (AuNPs) as the receptors to provide differential protein affinity and, hence, discrimination. In practice, cationic AuNPs electrostatically bind the anionic β -Gal, inhibiting the enzyme without denaturation.²⁵ Displacement of the particle by analyte proteins restores β -Gal activity, generating a fluorescent readout signal (Figure 1) that is amplified through enzymatic catalysis.

Results and Discussion

The anionic tetrameric enzyme β -Gal (17.5 \times 13.5 \times 9 nm, pI = 4.6, M_w = 465 kDa) was chosen as the amplifying element

- (24) Giljohann, D. A.; Mirkin, C. A. *Nature* **2009**, *462*, 461.
- (25) (a) De, M.; You, C.-C.; Srivastava, S.; Rotello, V. M. *J. Am. Chem. Soc.* **2007**, *129*, 10147. (b) Hong, R.; Fisher, N. O.; Verma, A.; Goodman, C. M.; Emrick, T.; Rotello, V. M. *J. Am. Chem. Soc.* **2004**, *126*, 739. (c) Jones, S.; Thornton, J. M. *Proc. Natl. Acad. Sci.* **1996**, *93*, 13. (d) W. Stites, E. *Chem. Rev.* **1997**, *97*, 1233. (e) Conte, L. L.; Chothia, C.; Janin, J. *J. Mol. Biol.* **1999**, *285*, 2177. (f) De, M.; Miranda, O. R.; Rana, S.; Rotello, V. M. *Chem. Commun.* **2009**, *16*, 2157.

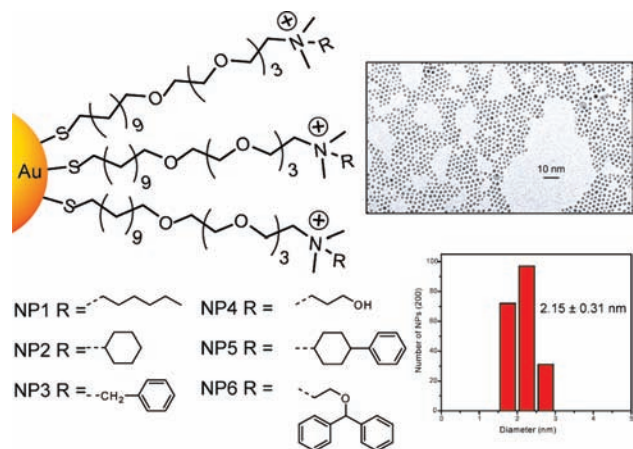


Figure 2. Structure features of the cationic gold nanoparticles (NP1–NP6). The transmission electron microscopy (TEM) and histogram plot show the morphology, monodispersity, and sizes of the metallic core gold nanoparticles.

due its stability to a wide range of temperature, pH, and ionic strength conditions.^{26,27} Gold nanoparticles (~2 nm core diameter) with a positive surface charge were used to bind efficiently to the anionic β -Gal through electrostatic complementary and electrostatic charge interactions (see Figures S29, S31, and S33 for zeta potential and DLS measurements). These particles feature a large surface area with size comparable to that of proteins, allowing these systems to mimic protein–protein surface interactions,²⁵ an excellent starting point for sensor design. These AuNPs feature a tetraethylene glycol unit in the ligand shell to minimize the denaturation of the bound enzyme/analyte protein and variable terminal functionality to generate the differential affinity required for sensing (Figure 2, Figure S29 and Table S7).²⁸

As a starting point, we focused on the optimization of the binding ratio between AuNPs (NP1–NP6) and β -Gal through inhibition activities in phosphate buffer. We conducted an activity assay of β -Gal-catalyzed hydrolysis at various concentrations of nanoparticles (see Figure S26). Typically, a concentration of 0.5 nM of β -Gal in phosphate buffer solution (5 mM, pH = 7.4) was incubated with various concentration of NP1–NP6 for 30 min, and 1 mM of the fluorogenic substrate (MUG, $\lambda_{\text{exc}} = 455$ nm) was added to the AuNP–enzyme complexes for the inhibition and enzyme–substrate reaction studies. As a control, the enzyme inhibition was also studied using neutral tetra(ethylene glycol)-functionalized nanoparticles. The normalized first-order rate of fluorogenic substrate hydrolysis was plotted versus the ratio of nanoparticles to β -Gal and showed a tendency to decrease upon addition of nanoparticles, as shown for NP2 in Figure 3. This result clearly indicates that activity of β -Gal is inhibited by nanoparticle binding. This inhibition of β -Gal activity depends on subtle structural changes of peripheral ligands on the AuNPs, with the linear end group (NP1) exhibiting less suppression than a branched isomeric

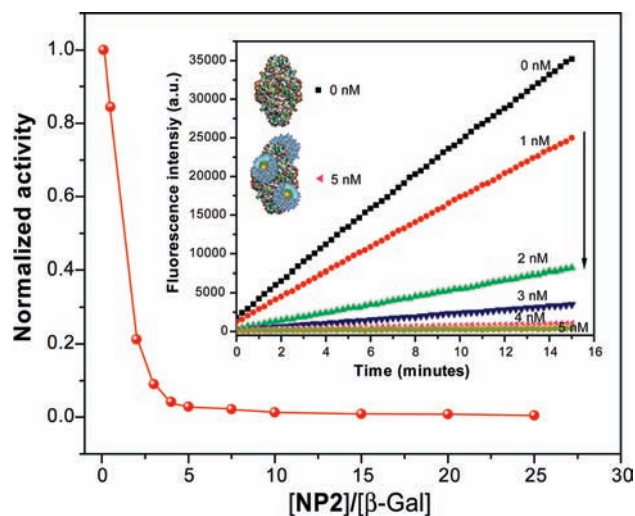


Figure 3. Normalized inhibition activity of β -Gal (0.5 nM) against 1 mM substrate MUG upon addition of cationic NP2 in 5 mM phosphate buffer. The inset shows the kinetics of the fluorescence spectra before and after addition of NP2. The arrow in the inset indicates the direction of activity (0 nM indicates free enzyme, and 5 nM indicates inhibited enzyme with NPs).

Table 1. Physical Properties of the Proteins Used As Sensing Targets in Phosphate Buffer Solution at pH 7.4^{18a}

protein ^a	M_w (kDa)	pI
<i>α-amylase (α-Am)</i>	50.0	5.0
bovine serum albumin (BSA)	66.3	4.8
cytochrome <i>c</i> (CytC)	12.3	10.7
<i>ferritin (Fer)</i>	750.0	4.5
human serum albumin (HSA)	69.4	5.2
<i>lipase (Lip)</i>	58.0	5.6
<i>lysozyme (Lys)</i>	14.4	11.0
<i>myoglobin (Myo)</i>	17.0	7.2
<i>alkaline phosphatase (PhosB)</i>	140.0	5.7

^a Proteins in *italics* are commonly found in human urine.

structure (NP2). Control experiments with noncharged NPs (NP_{TEG}) were carried out, and no interaction or inhibition of the enzyme was observed (see Figure S35).

A total of nine proteins of various sizes, surface charges, molecular weights, and isoelectric points were chosen to test generality and limitations of our sensor (Table 1, see Table S6 for zeta potentials, r_h values, and extinction coefficients at 280 nm of the analyte proteins). Fluorogenic substrate hydrolysis for the β -Gal/AuNP conjugates against individual proteins in buffer is summarized in Figure 4. The individual target proteins generated distinguishable and highly reproducible rates of the fluorogenesis, indicating the potential for protein discrimination.

All proteins were tested using a fluorescence displacement assay of six β -Gal/AuNP assemblies array for six replicate measurements, providing a data set as a $6 \times 6 \times 9$ matrix. The resulting data were analyzed through linear discrimination analysis (LDA) using SYSTAT software (version 11)²⁹ and transformed into five canonical factors. This statistical analysis method is used to recognize the linear combination of features that differentiate two or more classes of objects or events. The five canonical factors contain 42.2%, 34.1%, 12.1%, 5.8%, and 4.9% of the variation, respectively. The canonical score plot of the first three factors is presented in Figure 5, where each dot represents the fluorescence response pattern of a single protein

(29) SYSTAT11.0; SystatSoftware: Richmond, CA, 2004.

- (26) (a) Jacobson, R. H.; Zhang, X. J.; Dubose, R. F.; Matthews, B. W. *Nature* **1994**, *369*, 761. (b) Craven, G. R.; Steers, E.; Anfinsen, C. B. *J. Biol. Chem.* **1965**, *240*, 2468. (c) Verma, A.; Simard, J. M.; Worrall, J. W. E.; Rotello, V. M. *J. Am. Chem. Soc.* **2004**, *126*, 13987.
- (27) (a) Fowler, A. V.; Zabin, I. *J. Biol. Chem.* **1978**, *253*, 5521. (b) Fowler, A. V.; Zabin, I. *J. Biol. Chem.* **1970**, *245*, 5032. (c) Wallenfels, K.; Weil, R. *Enzymes*, 3rd ed.; 1972; Vol. 7, p 617.
- (28) (a) Hong, R.; Fischer, N. O.; Verma, A.; Goodman, C. M.; Emrick, T.; Rotello, V. M. *J. Am. Chem. Soc.* **2004**, *126*, 739. (b) Nikolic, M. S.; Krack, M.; Aleksandrovic, V.; Kornowski, A.; Förster, S.; Weller, H. *Angew. Chem.* **2006**, *118*, 6727.

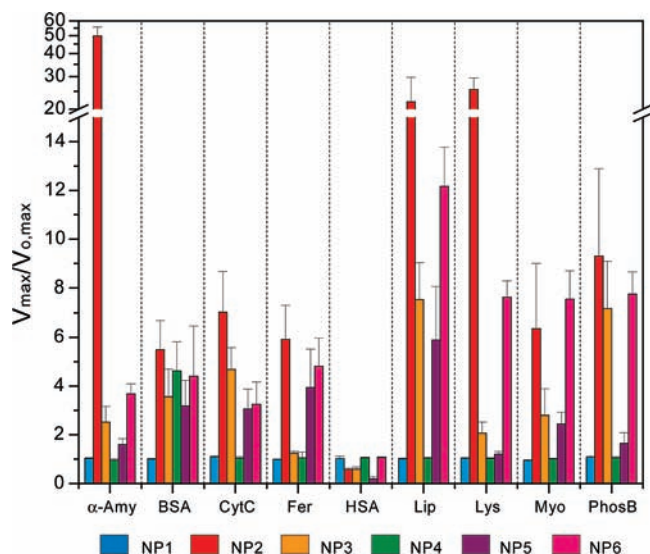


Figure 4. Fluorescence response patterns ratio of β -Gal and six AuNP adducts against various target proteins. Each value represents an average of six parallel measurements with standard deviation.

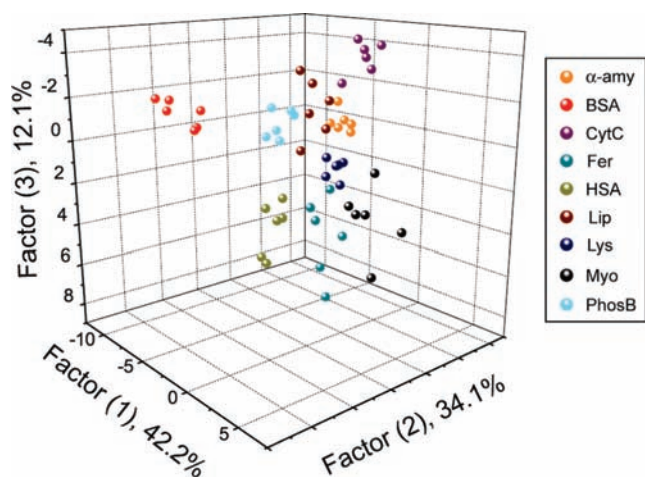


Figure 5. Canonical score plot of the first three factors of fluorescence response patterns obtained through β -Gal/AuNP sensor array against nine target proteins in 1 nM concentration.

target to the β -Gal/AuNP sensor array. The canonical plot reveals nine distinct clusters corresponding to individual target proteins that give rise to a 100% classification accuracy obtained from a jackknifed matrix in LDA. This result demonstrates that the β -Gal/AuNP sensor array is sensitive enough to differentiate target proteins in the 1 nM range, significantly more sensitive than prior methods (1–350 μ M),^{16,17,18c} including our previous fluorescent polymer–nanoparticle conjugates system (215 nM for the low M_w proteins).²¹

The high sensitivity of our β -Gal/AuNP sensor array can be attributed to signal amplification through the enzyme–substrate reaction of β -Gal. Significantly, the same training matrix analyzed using only one nanoparticle structure gives rise to classification accuracies of 33%, 44%, 37%, 31%, 44%, and 35% for NP1 to NP6, respectively, indicating almost equal ability of each particle to discriminate between protein targets (Table S3).

To investigate the robustness identification accuracy of the β -Gal/AuNP sensor array, we prepared 60 unknown protein samples at 1 nM randomly chosen from the training set for identification. The fluorescence response patterns obtained for

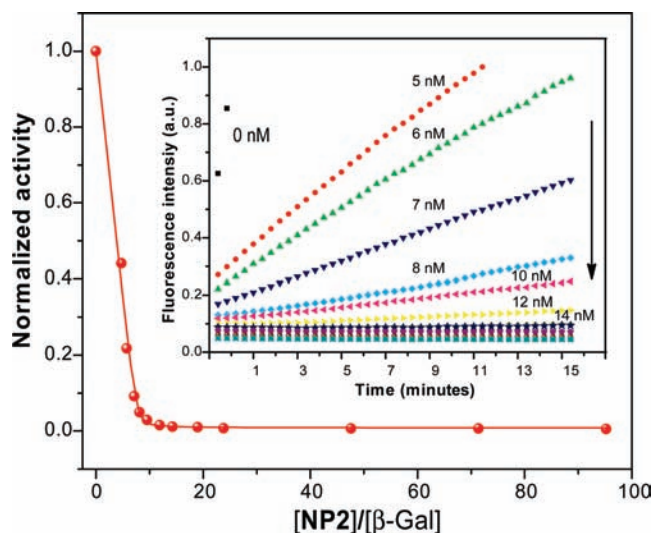


Figure 6. Normalized inhibition activity of β -Gal (0.5 nM) against 1 mM substrate MUG upon addition of cationic NP2 in the presence of desalted human urinary proteins. The inset shows the kinetics of the fluorescence spectra before and after addition of NP2. The arrow in the inset indicates the direction of activity.

each unknown against the sensor array were analyzed through LDA. The resulting patterns were classified through the canonical score plot by the first two factors of simplified fluorescence patterns based on the Mahalanobis distances of unknowns to the centroid of the respective protein clusters in the canonical score plot. An identification accuracy of 92% (55 correct out of 60) demonstrates reproducibility of our enzyme–nanoparticle sensor system for identification.

Sensing of proteins in real-world biofluids such as protein in human urine provides a far more demanding test than sensing in simple buffer solutions. The overall protein content (>1.5 μ M, 0.150 g/L) and the multianalyte nature of human urine (>1500 proteins as competing biomolecules) generate a complex matrix that is challenging for sensor design.³⁰ An additional complication is variation in ionic strength, an issue that is addressed biomedically through desalting using spin column chromatography. We employed this technique in our studies, but we are aware that as with current analytical methods this desalting adds an additional step to the analytical procedure (see Figures S27 and S28).^{30,31}

The complexation between β -Gal and cationic AuNPs in desalted human urine (Bioreclamation Inc.) was determined by the hydrolysis of MUG by β -Gal in the presence of various concentrations of AuNPs (Figure 6, additional information see Figures S34 and S35). In this experiment, β -Gal was dissolved in desalted human urine (\sim 1.5 μ M, see SI for details) buffered to pH = 7.4 using 5 mM phosphate buffer. This solution was then equilibrated with a stoichiometric amount of nanoparticles

(30) (a) Adachi, J.; Kumar, C.; Zhang, Y.; Olsen, J. V.; Mann, M. *Genome Biol.* **2006**, *7* (9), R80. (b) Li, S.-J.; Peng, M.; Li, H.; Liu, B.-S.; Wang, C.; Wu, J.-R.; Li, Y.-X.; Zeng, R. *Nucleic Acids Res.* **2009**, *37*, D907. (c) Fliser, D.; Novak, J.; Thongboonkerd, V.; Argilés, A.; Jankowski, V.; Girolami, M. A.; Jankowski, J.; Mischa, H. *J. Am. Soc. Nephrol.* **2007**, *18*, 1057.

(31) (a) Magistrini, R.; Ligabue, G.; Lupo, V.; Furci, F.; Leonelli, M.; Manganelli, L.; Masellis, M.; Gatti, V.; Cavazzini, F.; Tizzanini, W.; Albertazzi, A. *Nephrol., Dial., Transplant.* **2009**, *24*, 1672. (b) Roden, A. C.; Lockington, K. S.; Trostrud, L. J.; Katzmann, J. A. *Am. J. Clin. Pathol.* **2008**, *130*, 141. (c) Nedelkolov, D.; Nelson, R. W. *Am. J. Kidney Dis.* **2001**, *38*, 481. (d) Bottini, P.; Almerinda, M.; Alves, R.; Garlipp, C. R. *Am. J. Kidney Dis.* **2002**, *39*, E2.

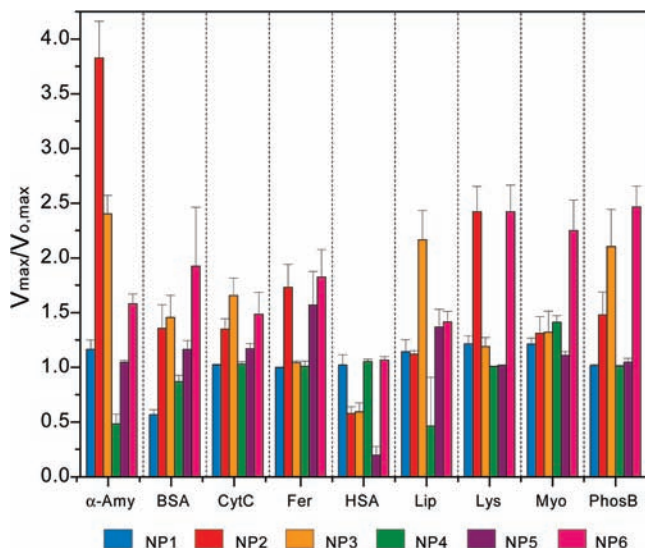


Figure 7. Fluorescence response patterns ratio of β -Gal and six AuNP adducts against various target proteins. Each value represents an average of six parallel measurements.

for 15 min. Then, an excess amount of the MUG solution (1 mM) was added to initiate the enzymatic reaction. The activity of β -Gal was directly correlated with the AuNP concentration, indicating that the activity of β -Gal is inhibited by AuNP complex formation.

Using the optimized conditions (*vide supra*), it was established that 1 nM concentration of spiked proteins was required for reproducible differentiation of the target analytes (Table 1). As before, we created a training matrix (six β -Gal/AuNP adducts \times nine proteins \times six replicates) with β -Gal/AuNP adduct and each of the proteins. Each protein in the human urine protein solution generated a distinct fluorescence response. The rates of fluorogenic substrate hydrolysis for the β -Gal/AuNP pair in the presence of individual protein analytes are summarized in Figure 7, showing that NP1 and NP4 exhibit stronger affinity for β -Gal than for other proteins, producing smaller hydrolysis rates and less fluorescence response. As before, this fluorescence response pattern was subjected to further LDA, producing a $6 \times 6 \times 9$ matrix. This matrix was transformed into five canonical factors. The five canonical factors contain 62.3%, 20.7%, 9.1%, 4.3%, and 0.9% of the variation, respectively.

The canonical score plot of the first three factors is presented in Figure 8, where each dot represents the fluorescence response pattern of a single protein target to the β -Gal/AuNP sensor array. The canonical plot reveals nine distinct clusters corresponding to individual target proteins, giving rise to a 100% classification accuracy based on the jackknifed matrix in LDA. This result demonstrates that the β -Gal/AuNP sensor array is sensitive enough to differentiate each of the target proteins at 1 nM in the biofluid matrix (0.067% of the total protein content in urine), comparable with the preliminary study carried out in buffer. This sensitivity is improved as described before, $4\text{--}2 \times 10^2$ -fold, in comparison with simple fluorophore displacement,²¹ and it is also comparable with the preliminary study carried out in buffer. The particles in this study are well suited for differentiation: the same training matrix analyzed using a single nanoparticle gives rise to classification accuracies of 33%, 52%, 41%, 43%, 48%, and 31% from NP1 to NP6, respectively (Table S10). This indicates an almost equal contribution of each particle in the discrimination of the examined protein targets.

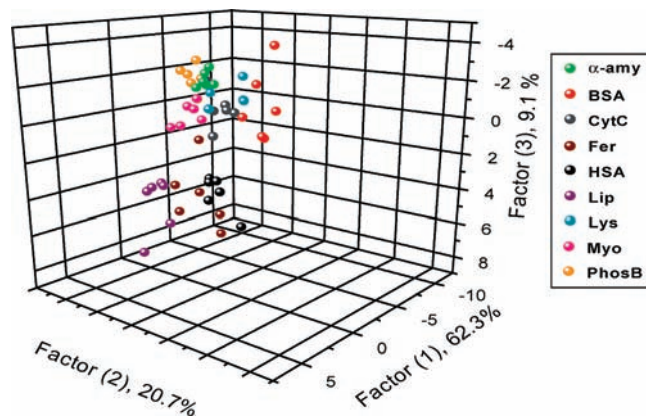


Figure 8. Canonical score plot of the first three factors of fluorescence response patterns ratio obtained through the β -Gal/AuNP sensor array against nine target proteins at 1 nM in desalted human urine ($\sim 1.5 \mu\text{M}$ total protein content).

The accuracy of the β -Gal/AuNP sensor array was validated by identifying unknown proteins in the competitive environment of the desalted human urine protein solution. Sixty unknown protein solutions spiked at 1 nM were chosen arbitrarily from the training set. The fluorescence response patterns were newly analyzed through LDA and further classified by the Mahalanobis distances of unknowns to the centroid of the respective protein clusters in the canonical score plot. This process identified 55 out of 60 unknowns correctly, corresponding to a 92% identification accuracy, demonstrating both the feasibility and reproducibility of our enzyme–nanoparticle sensor system.

Conclusions

In this study, we have demonstrated that the use of enzymatic amplification dramatically increases the sensitivity of the array-based sensing of proteins. Using this EAAS method, we rapidly and reproducibly sensed proteins at concentrations of 1 nM in both phosphate buffer and desalted human urine. These studies demonstrate that sensing can be achieved with high sensitivity in a complex biomatrix, providing an important first step for the creation of array-based biosensors for real-world diagnostic applications. In our ongoing studies, we are exploiting both new alternative approaches for protein detection and new data analysis strategies to apply this methodology to more complex matrices featuring a large diversity of target analytes.

Acknowledgment. This work was supported by the NSF Center for Hierarchical Manufacturing at the University of Massachusetts Nanoscale Science and Engineering Center (NSEC, DMI-0531171), the NSF (V.M.R., CHE-0808945), and the NIH (GM077173). U.H.F.B. thanks the Department of Energy Grant for generous financial support (DE-FG02-04ER46141).

Note Added after ASAP Publication. Typographical errors in the Supporting Information and an incorrect reference 26, published ASAP on March 23, 2010, have been corrected. The revised version was reposted April 14, 2010.

Supporting Information Available: Experimental section, synthesis of ligands, synthesis of gold nanoparticles, ^{13}C NMR and ^1H NMR spectra, fluorescence titration curves, training matrix, protein purification, gel electrophoresis, zeta potential, and dynamic light scattering. These materials are available free of charge via the Internet at <http://pubs.acs.org>.

JA1006756