



Speciation of arsenic in a thermoacidophilic iron-oxidizing archaeon, *Acidianus brierleyi*, and its culture medium by inductively coupled plasma–optical emission spectroscopy combined with flow injection pretreatment using an anion-exchange mini-column

Naoki Higashidani^a, Takashi Kaneta^{a,*}, Nobuyuki Takeyasu^a, Shoji Motomizu^b, Naoko Okibe^c, Keiko Sasaki^c

^a Department of Chemistry, Graduate School of Natural Science and Technology, Okayama University, 3-1-1 Tsushimanaka, Okayama 700-8530, Japan

^b Okayama University, 1-1-1 Tsushimanaka, Okayama 700-8530, Japan

^c Department of Earth Resources Engineering, Graduate School of Engineering, Kyushu University, 744 Motoooka, Fukuoka 819-0395, Japan

ARTICLE INFO

Article history:

Received 17 December 2013

Received in revised form

24 January 2014

Accepted 27 January 2014

Available online 3 February 2014

Keywords:

Thermoacidophilic iron-oxidizing archaeon

Acidianus brierleyi

Arsenic

Speciation

Inductively coupled plasma–optical emission spectroscopy

Flow injection pretreatment

ABSTRACT

The thermoacidophilic iron-oxidizing archaeon *Acidianus brierleyi* is a microorganism that could be useful in the removal of inorganic As from wastewater, because it simultaneously oxidizes As(III) and Fe(II) to As(V) and Fe(III) in an acidic culture medium, resulting in the immobilization of As(V) as FeAsO₄. To investigate the oxidation mechanism, speciation of the As species in both the cells and its culture media is an important issue. Here we describe the successive determination of As(III), As(V), and total As in *A. brierleyi* and its culture medium via a facile method based on inductively coupled plasma–optical emission spectroscopy (ICP–OES) with a flow injection pretreatment system using a mini-column packed with an anion-exchange resin. The flow-injection pretreatment system consisted of a syringe pump, a selection valve, and a switching valve, which were controlled by a personal computer. Sample solutions with the pH adjusted to 5 were flowed into the mini-column to retain the anionic As(V), whereas As(III) was introduced into ICP–OES with no adsorption on the mini-column due to its electrically neutral form. An acidic solution (1 M HNO₃) was then flowed into the mini-column to elute As(V) followed by ICP–OES measurement. The same sample was also subjected to ICP–OES without being passed through the mini-column in order to determine the total amounts of As(III) and As(V). The method was verified by comparing the results of the total As with the sum of As(III) and As(V). The calibration curves showed good linearity with limits of detection of 158, 86, and 211 ppb for As(III), As(V), and total As, respectively. The method was successfully applicable to the determination of the As species contained in the pellets of *A. brierleyi* and their culture media. The results suggested that the oxidation of As(III) was influenced by the presence of Fe(II) in the culture medium, i.e., Fe(II) enhanced the oxidation of As(III) in *A. brierleyi*. In addition, we found that no soluble As species was contained in the cell pellets and more than 60% of the As(III) in the culture medium was oxidized by *A. brierleyi* after a 6-day incubation.

© 2014 Elsevier B.V. All rights reserved.

1. Introduction

Arsenic (As) is an element that is known to be toxic to humans, but the degree of toxicity depends on whether the chemical species are classified as inorganic or organic [1,2]. The inorganic species include arsenite (As(III)) and arsenate (As(V)), which are known to be more toxic than the organic species such as monomethylarsinic acid and dimethylarsinic acid. Among these species, As(III) is the most toxic, followed by As(V) and the organic

varieties. Therefore, the speciation of the As species, particularly of the inorganic species, is an important issue in environmental chemistry, in earth resource engineering, and in the mining industry.

When determining the speciation of inorganic As, the simultaneous determination of three species, As(III), As(V), and total As, enhances the reliability of the results. Ordinarily, speciation is performed by the determination of two of the three As species. Several separation techniques such as high-performance liquid chromatography (HPLC) [3], ion chromatography (IC) [4,5], and capillary electrophoresis [6–8] were coupled using either inductively coupled plasma–optical emission spectroscopy (ICP–OES) or inductively coupled plasma–mass spectroscopy (ICP–MS) to

* Corresponding author. Tel./fax: +81 86 2517847.

E-mail address: kaneta@okayama-u.ac.jp (T. Kaneta).

achieve a sensitive determination of As(III) and As(V), whereas voltammetry was utilized for the determination of As(III) and total As, which must be determined after the chemical reduction of As(V) [9,10]. The separation of As(III) and As(V) requires an extended amount of time for analysis (approximately 10 to 30 min). Furthermore, sequential injections of biological samples may degrade the performance of the separation column for HPLC and IC since the adsorption of biological molecules such as proteins, lipids, and DNA should rapidly deteriorate the column. Compared to chromatographic methods, an automated flow injection system with solid-phase extraction has shown promise for reducing the analysis time and for solving the problem of damage to the analytical columns. For example, Jitmanee et al. have demonstrated a method for the speciation of As(III) and As(V) by ICP–OES coupled with a pretreatment system using two mini-columns to concentrate both As species, As(III) and As(V) [11]. This method was verified when it was used to determine the content of As(III) and As(V) in natural river water.

A convenient method for As speciation was important in the study of As immobilization using microorganisms. Okibe and coworkers reported that the microorganism would be useful for the immobilization of As species from acidic refinery wastewater via the simultaneous oxidation of As(III) and Fe(II) to As(V) and Fe(III) followed by the formation of insoluble species consisting of Fe(III) and As(V) using *Acidianus brierleyi* [12]. They demonstrated that the microorganism would be useful for the removal of As from the refinery wastewater that is produced in the mining industry, although the details surrounding the oxidation mechanism of *A. brierleyi* remain unclear. In their research, As species in the culture media were determined via voltammetry and ICP–OES, i.e., As(III) and total As were determined independently by voltammetry and ICP–OES, respectively. Therefore, a simple and easy method for the determination of the As species not only in culture media but also on cells would be attractive and useful in the study of the oxidation mechanism in *A. brierleyi*.

In the present study, we developed a method for the speciation of As by ICP–OES coupled with a flow injection pretreatment system using a single anion-exchange mini-column. The flow injection system consisted of a syringe pump, a selection valve, and a switching valve, which were controlled by a personal computer. Sample solutions were introduced into ICP–OES with and without passing through an anion-exchange mini-column to determine As(III), As(V), and total As in succession. The results obtained by the proposed method were more reliable than the other speciation methods since the total concentration was also determined simultaneously and could be directly compared with the determined concentrations of As(III) and As(V).

The developed method is facile, high-throughput, sensitive, selective, and reliable for the speciation of As and is applicable to the speciation of As in *A. brierleyi* and its culture media after different incubation times. To the best of our knowledge, this is the first report concerning the determination of the As species in *A. brierleyi* cells. Therefore, the method for speciation of microorganisms has been successfully proven to work using *A. brierleyi* in this study. The results for the culture media were consistent with a previous report by Okibe and coworkers [12]. In addition, we found that As(III) was completely oxidized and immobilized in the microorganism after a 6-day incubation.

2. Experimental

2.1. Materials

All reagents were of analytical grade and were used without further purification. All solutions were prepared by being dissolved

in water that had been purified by means of an ultrapure MILLI-Q system (Millipore, Molsheim, France). Stock solutions of As(III) and As(V) (1000 mg L^{-1}) were prepared by dissolving sodium arsenite (NaAsO_2) and disodium hydrogen arsenate heptahydrate ($\text{Na}_2\text{HAsO}_4 \cdot 7\text{H}_2\text{O}$), which were obtained from Nacalai tesque, Inc. (Kyoto, Japan). A standard solution of 1000 mg L^{-1} Fe(III) (iron(III) nitrate in 0.1 M nitric acid), sodium acetate, iron(II) sulfate heptahydrate, and ammonium iron(II) sulfate hexahydrate were purchased from Wako pure chemicals (Osaka, Japan). A stock solution of Fe(II) was prepared by dissolving ammonium iron(II) sulfate hexahydrate in water with the addition of a small amount of sulfuric acid (Electronic grade, Mitsubishi chemicals, Tokyo, Japan). The stock solutions were diluted daily in order to prepare standard solutions for constructing calibration curves. A 0.1 M sodium acetate solution was used as a preconditioning solution for the mini-column packed with anion-exchange resin (Wako DOWEX 1×4 50–100 Mesh, Wako pure chemicals, Osaka, Japan). An acetate buffer solution (pH 5.0) was prepared by mixing 0.1 M acetic acid (Electronic grade, Kanto chemical Co. Inc, Tokyo, Japan) and 0.1 M sodium acetate solutions and the pH was monitored using a pH meter D-52 (HORIBA, Ltd., Kyoto, Japan). Nitric acid (electronic grade) was obtained from Mitsubishi chemical (Tokyo, Japan).

2.2. Sample preparation

The microorganisms used in this study, *A. brierleyi* (DSMZ 1651), were cultured in the same manner as that reported in a previous paper [12,13]. Briefly, *A. brierleyi* was cultured in a 500 mL Erlenmeyer flask containing 200 mL of 9 K basal salts medium (pH was adjusted to 1.5 with H_2SO_4) with 500 mg L^{-1} As(III) in either the presence or absence of 900 mg L^{-1} Fe(II) as $\text{FeSO}_4 \cdot 7\text{H}_2\text{O}$. The microorganisms were incubated at 70°C with shaking at 100 rpm. The culture medium was centrifuged to separate the microorganisms, which were then collected for the measurement of the As species.

Under these conditions, the number of cells was observed to decrease [12], which was attributed to both a lack of an energy source and the toxicity of As(III) to *A. brierleyi*. However, As(III) was only weakly toxic, since the *A. brierleyi* culture was still alive even after 14-days incubation although a gradual decrease in the number of cells was observed [12].

For the preparation of the culture medium samples, 0.25 mL of culture medium was diluted to 5 mL by the addition of 2.5 mL of 0.1 M acetate buffer to adjust the pH to 5.0, which resulted in a 500-fold diluted culture medium sample solution containing 10 mM acetate buffer. The cell pellets were dissolved with 0.5 mL of B-PER, protein extraction reagents (Thermo Fisher Scientific, USA), and 0.5 mL of 0.1 M acetate buffer was added to the solution to adjust the pH to 5.0. Then, the solution was diluted with water to a total volume of 5 mL. Throughout the experiments, all sample solutions were filtered using $0.45 \mu\text{m}$ membrane filters (mixed cellulose ester, DISMIC-25_{AS}, Advantec, Tokyo, Japan).

2.3. Apparatus

An ICP–OES (Vista Pro, Seiko Instrument & Varian Instrument) was used for the determination of the As species under conditions recommended by the manufacturer. A laboratory-built pretreatment system, Auto-Pret, was employed for the successive measurements of As(III), As(V), and their total concentrations. The system has been reported in previous papers [14–16]. Briefly, the system consisted of a syringe pump, an 8-port selection valve, and a 6-port switching valve, all of which were controlled by a personal computer using in-house software written by Visual Basic.

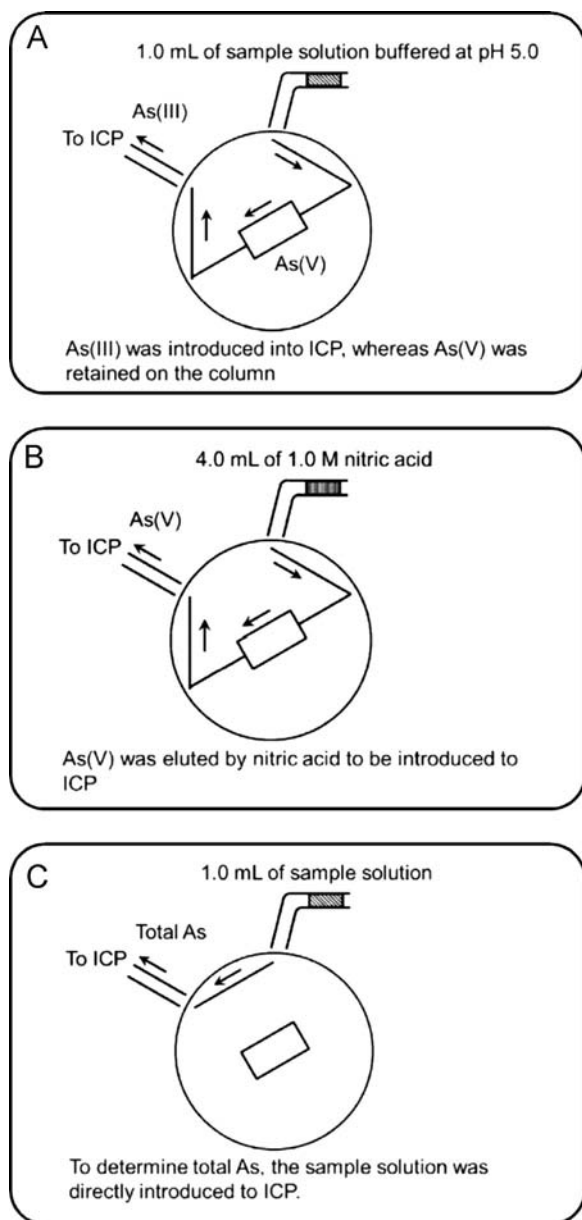


Fig. 1. Flow diagram for the determination of As(III), As(V) and their total. (A) Introduction of As(III) to ICP-OES, (B) introduction of As(V) to ICP-OES, and (C) introduction of total As to ICP-OES.

A mini-column (2 mm i.d. \times 40 mm, polypropylene) that was produced in-house was packed with anion-exchange resin and was connected to the selection valve of the Auto-Pret. A schematic illustration of the flow diagram is shown in Fig. 1. Initially, the mini-column was preconditioned with 4 mL of 0.1 M sodium acetate solution. Then, 1 mL of a sample solution buffered at pH 5 was introduced into the mini-column where As(III) was separated from As(V) when the As(V) was retained onto anion-exchange resin (Fig. 1(A)). The mini-column was then washed with 3 mL of water for transport of the As(III) to ICP-OES. After the measurement of the As(III), 4 mL of 1 M HNO₃ was introduced into the mini-column to elute and transport the As(V) to ICP-OES (Fig. 1(B)). Finally, the switching valve was switched so the sample would not pass through the mini-column and another 1 mL of the sample was subjected to ICP-OES to determine the total concentration of As (Fig. 1(C)). The data obtained via ICP-OES, i.e., the charts of time (s) vs. intensity (cps), were processed via ICP-OES

Instrument Software V4.0 (Seiko Instruments, Chiba, Japan) and an in-house LabVIEW program.

3. Results and discussion

3.1. Optimization of the pH for the sample and eluent

The separation of As(III) and As(V) was easily achieved by anion-exchange resin since the acid dissociation constants, pK_{a1} , of As(III) (arsenite) and As(V) (arsenate) were 9.22 and 2.22, respectively [17]. Accordingly, the As(III) had no charge in the pH range of 0–7, whereas more than 99% of the As(V) was anionic with a pH of more than 4.22. Therefore, if the pH of a sample was adjusted to 5 with acetate buffer, only As(III) would pass through the anion-exchange column due to the selective adsorption of As(V). After the As(III) had passed through the column, the As(V) could be eluted via the sequential flowing of an acidic solution. Conversely, to determine the total As, we switched the switching valve so that the sample would not pass through the mini-column, which resulted in a direct introduction of the sample into ICP-OES.

For quantitative analysis of the As species, the pH of the sample solution and the concentrations of the nitric acid used as an eluent for As(V) were varied for optimization. The pH of the sample solution containing As(III) and As(V) was adjusted using 0.1 M acetate buffer solutions with different pH values. At pH values of 4 to 6, the peak areas for As(III) were constant, i.e., As(V) was completely retained on the mini-column even at pH 4. The nitric acid solutions with concentrations that differed from 0.1 to 2 M were examined in order to elute the As(V) that had been retained on the anion-exchange resin. The results showed that a concentration of more than 1 M was sufficient to elute the As(V) from the mini-column. Consequently, the pH values of the sample solutions were adjusted to 5.0 using the acetate buffer, then 1.0 M of nitric acid was employed to elute the As(V) that had been retained on the anion-exchange resin. The measurements of the As(III), As(V), and total As are summarized in Table 1. As shown in Table 1, the flow rate was optimized at $30 \mu\text{L s}^{-1}$ (1.8 mL min^{-1}), for which the total analysis time of one sample, including the preconditioning step, was about 16 min.

The present method has the following advantages; the instrument is much simpler than HPLC, three species (As(III), As(V) and their total) are simultaneously determined, replacement of a packing material is easy because of no need of high pressure for packing, and successive measurements are automated by a program. So, the pretreatment system provides inexpensive, reliable, and rapid analytical method for As speciation.

3.2. Calibration curves

For the determination of each As species, calibration curves of As(III), As(V), and total As were constructed under the optimized conditions described in Section 3.1. The typical signals of the flow analysis are shown in Fig. 2. The sample solutions contained 0.2, 0.4, and 1.0 ppm of As(III) and As(V) so that the totals were 0.4, 0.8, and 2.0 ppm, respectively. Fig. 2 shows the three consecutive peaks of As(III) and As(V) with the totals in the same order. As noted in Fig. 2, As(V) was detected as sharp peaks since it was concentrated on the mini-column. Conversely, the peak width for As(III) and the totals were broader than that of As(V) due to the lack of preconcentration in the mini-column. The standard solutions with different concentrations of As(III) and As(V) were measured to construct the calibration curves, and the results are summarized in Table 2. At the concentration range of 0–1.0 ppm, each calibration curve showed good linearity, while the slopes were different. The change in the slopes of the calibration curves

Table 1
Operation program for As speciation.

Steps	Pump valve	Selection valve	Switching valve*	Volume (μL)	Flow rate ($\mu\text{L s}^{-1}$)
Column washing (Water)	Aspirate	In	1	1000	100
	Dispense	Out		5	30
Column conditioning (Sodium acetate)	Aspirate	2	1	4000	100
	Dispense	5		4000	30
Column washing (Water)	Aspirate	In	1	4000	100
	Dispense	Out		5	30
Sample loading (Sample)	Aspirate	3	1	1000	100
	Dispense	5		4000	30
Eluent (Nitric acid)	Aspirate	4	1	4000	100
	Dispense	5		4000	30
Washing (Water)	Aspirate	In	2	4000	100
	Dispense	Out		5	30
Total As (Sample)	Aspirate	3	2	1000	100
	Dispense	5		4000	30

* Switching Valve Position: 1; passing through the mini-column, 2; flowing to the ICP-OES directly.

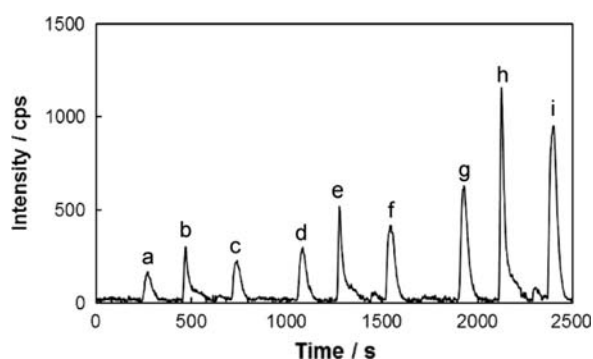


Fig. 2. Typical profiles of flow analysis. *a*=0.2 ppm As(III), *b*=0.2 ppm As(V), *c*=0.4 ppm As, *d*=0.4 ppm As(III), *e*=0.4 ppm As(V), *f*=0.8 ppm As, *g*=1.0 ppm As(III), *h*=1.0 ppm As(V), *i*=2.0 ppm As. The details of the experimental conditions are given in the text.

Table 2
Calibration curves for As species.

Species	Concentration range (ppm)	Regression curve*	Correlation coefficient (R^2)
As(III)	0–1.0 (0.2 intervals)	$y=95.8x$	0.9937
As(V)	0–1.0 (0.2 intervals)	$y=129x$	0.9843
Total	0–2.0 (0.4 intervals)	$y=80.3x$	0.9986

* The regression curves were obtained by fixing origin since no blank signal was observed for the sample without As.

were attributed to the change in the flow rate of each solution when introduced into ICP-OES, and to the preconcentration of As(V) by the mini-column. In terms of the flow rate, we confirmed that the slope of the calibration curve was reduced as the flow rate was increased. Although the flow rate was always controlled at $30 \mu\text{L s}^{-1}$, the mini-column increased the pressure, which resulted in a slightly decreased flow rate. Therefore, during the measurement of total As, the flow rate was faster than it was for the As(III) and As(V) measurements, resulting in a slope for total As that was smaller than that for As(III). Conversely, the difference in the slopes between As(III) and As(V) was attributed to the preconcentration of As(V) on the mini-column. The limits of detection (LOD) for the As species (defined as the concentrations at a signal-to-noise ratio=3 where the noise was defined as the standard deviation of the background signals over a distance equal to 20 times the width at half-height of the peak [18]) were estimated to be 158 ppb for As(III), 86 ppb for As(V) and 211 ppb for total As.

The LODs were slightly higher than those reported in the previous publications, e.g., 10 ppb for As(III) and As(V) in HPLC-ICP-OES [3] and 0.1 ppb for As(III) and As(V) in ICP-OES coupled with a preconcentration system [11]. However, the LODs obtained in the present method were low enough to determine the concentrations of the As species in the culture media of *A. brierleyi*.

3.3. Precipitation formation between As and Fe

Scordite, $\text{FeAsO}_4 \cdot 2\text{H}_2\text{O}$, is insoluble in water and its solubility product is $10^{-21.7}$ [19]. Therefore, when *A. brierleyi* produced Fe(III) and As(V), scordite or scordite-like ferric arsenate was simultaneously formed in the microorganisms, resulting in the immobilization of As species. To confirm the precipitation formation under the present culture conditions, 0–900 ppm of Fe(III) or Fe(II) solution was added to a mixture containing 200 ppm As(III) and 200 ppm As(V), respectively. Before the ICP-OES measurements, the sample solutions containing different concentrations of Fe(II) or Fe(III) were diluted 500-fold with the addition of 0.1 M acetate buffer. The concentration of each As species was plotted against the concentrations of Fe added to the samples, as shown in Fig. 3. When Fe(III) was added to the mixture of As(III) and As(V), the concentration of As(V) was gradually decreased as the concentration of Fe(III) was increased due to the formation of precipitation between As(V) and Fe(III), while the concentration of As(III) was constant (Fig. 3(A)). Thus, the decrease in the total As concentration meant a selective precipitation of As(V) with Fe(III). Conversely, the concentrations of all As species remained constant when Fe(II) was added to the As mixture (Fig. 3(B)), i.e., no precipitation was formed in the presence of Fe(II). This means that the As and Fe must be As(V) and Fe(III) in order to form a precipitation of As and Fe as expected from the small solubility product of scordite.

3.4. Effect of Fe(II) on the oxidation of As(III) by *A. brierleyi*

Okibe and coworkers have demonstrated that the oxidation of As(III) to As(V) was enhanced in the presence of Fe(II), i.e., As(III) and Fe(II) were simultaneously oxidized by *A. brierleyi*, followed by the immobilization as precipitation of Fe(III) and As(V). *A. brierleyi* can oxidize Fe(II) to Fe(III) in its growth process, whereas the rate of the redox reaction between Fe(III) and As(III) was too small to detect As(V) in a medium containing Fe(III) [12] although Fe(III) can oxidize As(III) to As(V), according to the standard redox potential for Fe(II)/Fe(III) and As(III)/As(V) [17]. Therefore, As(III) should also be oxidized by *A. brierleyi*, as proposed by Okibe et al. [12]. To confirm this simultaneous oxidation, two kinds of culture

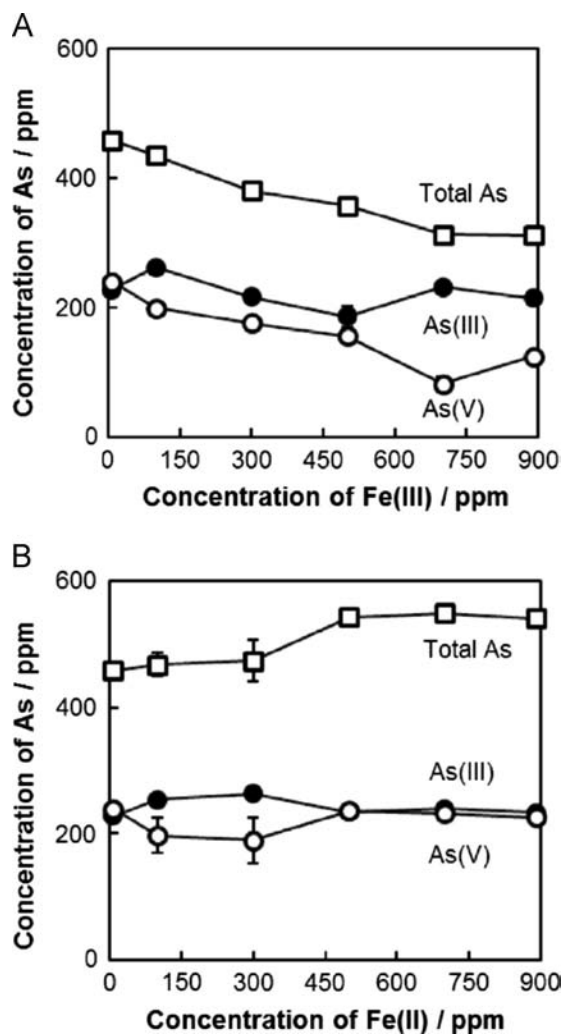


Fig. 3. Effect of iron on the precipitation of As species. The samples contained 200 ppm As(III) and 200 ppm As(V). (A) Addition of Fe(III), (B) addition of Fe(II). Other conditions are given in the text.

media containing 500 ppm of As(III) were prepared, one with 900 ppm of Fe(II) and another without Fe(II). After incubating *A. brierleyi* for 14 days, the concentrations of the As species in each medium were determined by the proposed method. The results are shown in Fig. 4: (A) without Fe(II) and (B) with Fe(II). In the absence of Fe(II), the peak area of As(III) was much larger than that of As(V), i.e., the oxidation of As(III) would not take place or would proceed very slowly in the culture medium. However, the peak area of As(V) increased as that of As(III) was decreased in the presence of Fe(II). The total As concentrations were in good agreement with the sum of As(III) and As(V) for both forms of culture media, that is, no loss of the As species was found in the pretreatment system. Therefore, these results support those obtained by Okibe and coworkers who found that the oxidation of As(III) by *A. brierleyi* was promoted by the presence of Fe(II) in the culture medium.

3.5. Determination of the As species in the culture media and *A. brierleyi* cells

In the presence of *A. brierleyi*, As(III) was immobilized by the simultaneous oxidation of As(III) and Fe(II) followed by the precipitation formation between As(V) and Fe(III). In addition, Fe(II) was needed for the oxidation of As(III) to As(V) by *A. brierleyi*, although the reason remains unclear. To obtain further

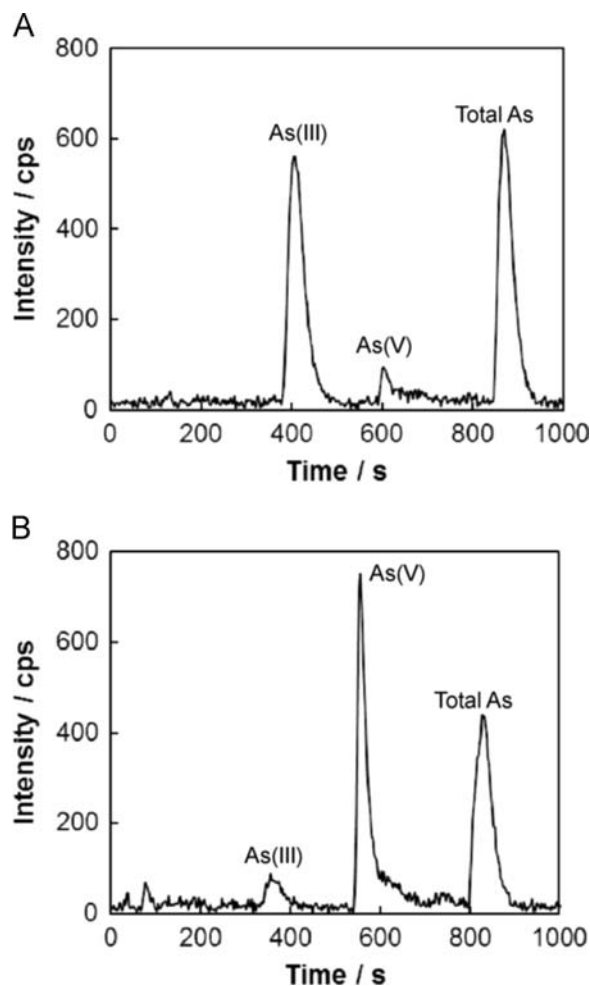


Fig. 4. Effect of Fe(II) on the oxidation of As(III) by *Acidianus brierleyi*. The culture medium samples contained 500 ppm As(III). The cells were incubated in the culture media (A) without Fe(II) and (B) with Fe(II). Other conditions are given in the text.

information on the oxidation process, we attempted to determine the As species in the culture media and the cell pellets at different incubation times. Fig. 5 shows the dependence on incubation time of the As(III), As(V), and total As concentrations in the media and cells. In the culture media, As(III) decreased rapidly and became constant after 6 days while As(V) was almost constant. Since only As(III) was dissolved in the culture medium before incubation, the decreased As(III) meant that the *A. brierleyi* had oxidized As(III) to As(V). The constant concentration of As(V) may be due to the exocytotic release of As(V) from the precipitation formed in the cells. A similar decrement of As(III) in the culture media was observed in a recent study by Okibe et al. although the residual amounts of As(III) were different from their results where As(III) was completely oxidized after a 6-day incubation [20]. A possible reason may be a different sample storage method, i.e., our samples were frozen for delivery in the present study while their samples were stocked in a refrigerator and were determined within one week.

It should be noted that the present study is the first demonstration of As speciation in *A. brierleyi* cells. The results of the cell pellets indicated that the As species in the cells was only As(V); i.e., As(III) was completely oxidized to As(V) in the cells after a 6-day incubation. The total As concentration was in good agreement with the sum of As(III) and As(V) so that each species was successfully determined by the proposed method. The results in Fig. 5(B) confirmed that As was completely immobilized in the

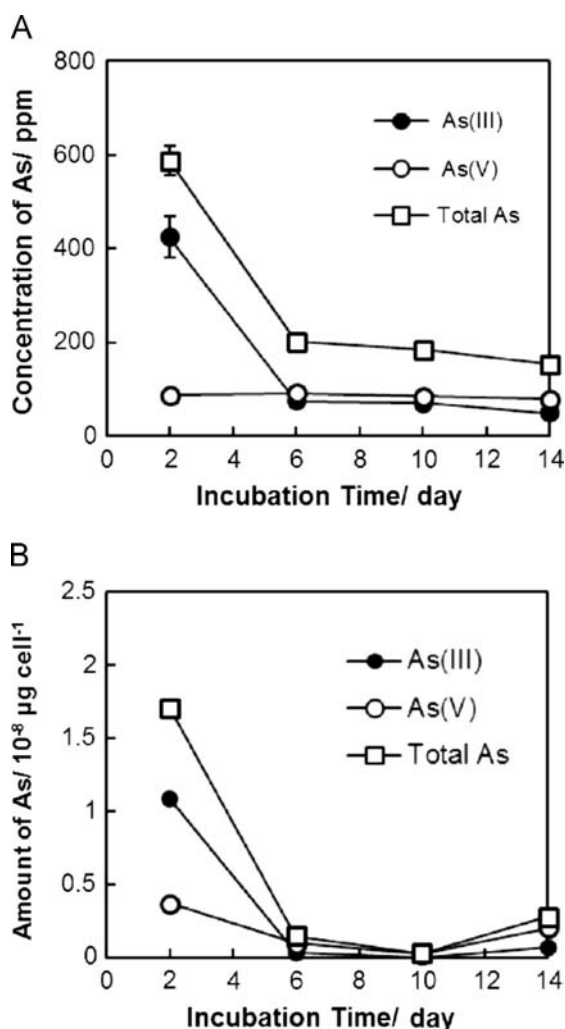


Fig. 5. Speciation of As in *A. brierleyi* and its culture medium at different incubation times. *A. brierleyi* was cultured in the media containing 500 ppm As(III) and 900 ppm Fe(II). The amounts of As in the cells were divided by the number of the cells in order to correct the effect of the differences in the cell population. Other conditions are given in the text.

cells after 6 days [19], because no As(III) and only trace amounts of As(V) were found in the cell pellets.

The concentration of As(V) in the culture medium was almost constant at 100 ppm after a 6-day incubation. The concentration was much lower than the solubility of scorodite under culture conditions of pH 1.0 since the solubility of scorodite has been estimated at more than 10 mM, which corresponds to 749 ppm [18]. Therefore, the precipitation of the ferric arsenate produced in *A. brierleyi* would be immobilized in the cell body and/or extracellular polymeric substances region without being exposed to the culture medium, as proposed by Okibe and coworkers [12]. The results for the cell pellets also supported the proposed mechanism since no As (or a trace amount) was found in the cell pellets after a 6-day incubation; i.e., As(III) was completely oxidized and was immobilized in the cell body and/or extracellular polymeric

substances region. Consequently, these results suggest that the proposed method is applicable to the speciation of the As species in *A. brierleyi* and its culture media.

4. Conclusion

Here we developed a facile and reliable method for the determination of As(III), As(V), and total As via ICP–OES coupled with a flow-injection pretreatment system using a mini-column packed with an anion-exchange resin. The method was successfully applicable to the speciation of As in *A. brierleyi* cells and its culture medium. The results obtained in this study support the simultaneous oxidation of As(III) and Fe(II) as proposed in a previous study. The results for the determination of As species in cell pellets indicated that As(III) was completely oxidized to As(V) in the cultured *A. brierleyi* after a 6-day incubation. This fact is consistent with a previous report, which mentioned that As was immobilized as As(V) in *A. brierleyi*. Therefore, ICP–OES coupled with a flow-injection pretreatment system is a useful technique in the study of the oxidation mechanism of *A. brierleyi*, which is promising for use in the treatment of industrial and natural water containing inorganic As species.

Acknowledgements

The authors gratefully thank the Division of Instrumental Analysis, Department of Instrumental Analysis & Cryogenics, Advanced Science Research Center, Okayama University for the ICP–OES measurements. A part of this research was supported by a Grant-in-Aid for Scientific Research (B) (No. 22350036) and a Grant-in-Aid for Exploratory Research (No. 25620114).

References

- [1] M.F. Hughes, *Toxicol. Lett.* 133 (2002) 1–16.
- [2] D.J. Thomas, *Environ. Geochem. Health* 16 (1994) 107–111.
- [3] M. Chausseau, C. Roussel, N. Gilon, J.M. Mermet, *Fresenius J. Anal. Chem.* 366 (2000) 476–480.
- [4] Y.L. Chu, S.J. Jieng, *J. Chromatogr. A* 1218 (2011) 5175–5179.
- [5] R.Y. Wang, Y.L. Hsu, L.F. Chang, S.J. Jieng, *Anal. Chim. Acta* 590 (2007) 239–244.
- [6] J.A. Day, K.L. Sutton, R.S. Soman, J.A. Caruso, *Analyst* 125 (2000) 819–823.
- [7] J.E. Prest, S.J. Baldock, P.R. Fielden, N.J. Goddard, B.J.T. Brown, *J. Chromatogr. A* 990 (2003) 325–334.
- [8] J.E. Prest, S.J. Baldock, P.R. Fielden, N.J. Goddard, B.J.T. Brown, *Microchim. Acta* 151 (2005) 223–230.
- [9] M. Esteban, C. Arino, I. Ruisanchez, M.S. Larrechí, F.X. Rius, *Anal. Chim. Acta* 285 (1994) 193–208.
- [10] K. Gibbon-Walsh, P. Salaün, C.M.G. van den Berg, *Anal. Chim. Acta* 662 (2010) 1–8.
- [11] K. Jitmanee, M. Oshima, S. Motomizu, *Talanta* 66 (2005) 529–533.
- [12] N. Okibe, M. Koga, K. Sasaki, T. Hirajima, S. Heguri, S. Asano, *Miner. Eng.* 48 (2013) 126–134.
- [13] M.P. Silverman, D.G. Lungren, *J. Bacteriol.* 77 (1959) 642–647.
- [14] H. Jin, A. Samarudin, M. Oshima, S. Motomizu, *Bunseki Kagaku* 58 (2006) 699–706.
- [15] R.K. Katarina, N. Lenghor, S. Motomizu, *Anal. Sci.* 23 (2007) 343–350.
- [16] O. Noguchi, M. Oshima, S. Motomizu, *Talanta* 78 (2009) 1235–1239.
- [17] G.D. Christian, *Analytical Chemistry*, fifth ed., John Wiley & Sons Inc., New York, Chichester, Brisbane, Toronto, Singapore, 1994.
- [18] R. Boqué, Y.V. Heyden, *LCGC Europe* 22 (2009) 82–85.
- [19] P.M. Dome, J.D. Rimstidit, *Am. Mineral* 70 (1985) 838–844.
- [20] N. Okibe, M. Koga, S. Moroshita, M. Tanaka, S. Heguri, S. Asano, K. Sasaki, T. Hirajima, *Hydrometallurgy* 143 (2014) 34–41.