

*TB 9-6625-2146-24

DEPARTMENT OF THE ARMY TECHNICAL BULLETIN

CALIBRATION PROCEDURE FOR AC AND DC VOLTMETERS AND AC AND DC AMMETERS (GENERAL)

Headquarters, Department of the Army, Washington, DC

7 January 2008

Distribution Statement A: Approved for public release; distribution is unlimited.

REPORTING OF ERRORS AND RECOMMENDING IMPROVEMENTS

You can improve this manual. If you find any mistakes or if you know of a way to improve these procedures, please let us know. Mail your letter or DA Form 2028 (Recommended Changes to Publications and Blank Forms) directly to: Commander, U.S. Army Aviation and Missile Command, ATTN: AMSAM-MMC-MA-NP, Redstone Arsenal, AL 35898-5000. A reply will be furnished to you. You may also send in your comments electronically to our E-mail address: 2028@redstone.army.mil or by fax 256-842-6546/DSN 788-6546. For the World Wide Web use: <https://amcom2028.redstone.army.mil>. Instructions for sending an electronic 2028 can be found at the back of this manual.

SECTION		Paragraph	Page
	I. IDENTIFICATION AND DESCRIPTION		
	Test instrument identification	1	2
	Forms, records, and reports.....	2	2
	Calibration description	3	2
	II. EQUIPMENT REQUIREMENTS		
	Equipment required.....	4	4
	Accessories required.....	5	4
	III. CALIBRATION PROCESS		
	Preliminary instructions.....	6	5
	Equipment setup	7	5
	Dc volts.....	8	6
	Dc amps.....	9	7
	Ac volts.....	10	9
	Ac amps.....	11	11
	Final procedure	12	13

*This bulletin supersedes TB 9-6625-2146-35, 14 February 1985, including all changes.

SECTION I IDENTIFICATION AND DESCRIPTION

1. Test Instrument Identification. This bulletin provides instructions for the calibration of Ac and Dc Voltmeters and Ac and Dc Ammeters listed in table 1. The manufacturers' manuals and/or TM's were used as the prime data sources in compiling these instructions. The equipment being calibrated will be referred to as the TI (test instrument) throughout this bulletin.

a. Model Variations. Variations among models are listed in the text.

b. Time and Technique. The time required for each calibration is approximately 1 hour, using the dc/low frequency technique.

2. Forms, Records, and Reports

a. Forms, records, and reports required for calibration personnel at all levels are prescribed by TB 750-25.

b. Adjustments to be reported are designated (R) at the end of the sentence in which they appear. When adjustments are in tables, the (R) follows the designated adjustment. Report only those adjustments made and designated with (R).

3. Calibration Description. TI parameters and performance specifications which pertain to this calibration are listed in table 1.

Table 1. Calibration Description

Test instrument		
Manufacturer and model	Parameters	Performance specifications
General Electric, Model AK-4	Ac volts	Range: 0 to 750 V Accuracy: $\pm 3\%$ FS at 60 Hz
	Ac amps	Range: 0 to 800 A Accuracy: $\pm 3\%$ FS at 60 Hz
Sensitive Research Instrument Corporation (SRI), Model C-CILKI (horizontal position)	Dc milliamps	Range: 0 to 100 mA Accuracy: $\pm 0.25\%$ of FS
Sensitive Research Instrument Corporation (SRI), Model C-CILORD (horizontal position)	Dc amps	Range: 0 to 30 A Accuracy: $\pm 0.25\%$ of FS
ME-221/U (horizontal position)	Dc milliamps	Range: 0 to 500 mA Accuracy: $\pm 0.5\%$ of FS
ME-489/U (clamp-on ammeter)	Ac volts	Range: 0 to 150, 300, 600 V Accuracy: $\pm 3\%$ of FS at 50 or 60 Hz
	Ac amps	Range: 0 to 6, 15, 60, 150, 300 A Accuracy: $\pm 3\%$ of FS at 50 or 60 Hz
ME-65/U and ME-65A/U (horizontal position)	Ac amps	Range: 0 to 200 A Accuracy: $\pm 0.5\%$ of FS, 20 to 500 Hz
Westinghouse, Model PA-5 (horizontal position)	Ac amps	Range: 0 to 200 A Accuracy: $\pm 0.5\%$ of FS, 20 to 135 Hz
Westinghouse, Model PY-4 Style 936-368 (horizontal position)	Ac volts	Range: 0 to 450 V Accuracy: $\pm 0.75\%$ of FS, 5 to 200 Hz

Table 1. Calibration Description - Continued

Test instrument		
Manufacturer and model	Parameters	Performance specifications
TS-340/U (horizontal position)	Ac volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS, 25 to 400 Hz
	Dc volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS
ME-79/USM-33	Ac volts	Range: 0 to 600 V Accuracy: $\pm 5\%$ of FS, 50 to 1000 Hz
	Ac amps	Range: 0 to 600 A Accuracy: $\pm 5\%$ of FS, 50 to 1000 Hz
TS-340/U (horizontal position)	Ac volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS, 25 to 400 Hz
	Dc volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS
TS-443/U (horizontal position)	Dc volts	Range: 0 to 150 V dc Accuracy: $\pm 0.25\%$ of FS
Weston, Model 155 (horizontal position)	Ac amps	Range: 0 to 50 A Accuracy: $\pm 0.5\%$ of FS, 25 to 500 Hz
Weston, Model 430 (horizontal position)	Dc amps	Range: 100 μ A to 50 A Accuracy: $\pm 0.5\%$ of FS
	Dc volts	Range: All ranges Accuracy: $\pm 0.5\%$ of FS
Weston, Model 433 (horizontal position)	Ac volts	Range: 0 to 750 V Accuracy: $\pm 0.75\%$ of FS, 25 to 125 Hz $\pm 1.25\%$ of FS, 125 to 2500 Hz
Weston, Model 455 (horizontal position)	Dc volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS
	Ac volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS, 25 to 1000 Hz
Weston, Model 538 (horizontal position)	Ac volts	Range: 0 to 600 V Accuracy: $\pm 2\%$ of FS, 25 to 125 Hz
	Ac amps	Range: 0 to 50 A Accuracy: $\pm 2\%$ of FS, 25 to 500 Hz
Weston, Model 622 Series (horizontal position)	Dc volts	Range: 0 to 1000 V Accuracy: $\pm 0.5\%$ of FS
	Dc amps	Range: 0 to 500 mA Accuracy: $\pm 0.5\%$ of FS
Weston, Model 633 Series (horizontal position)	Ac volts	Range: 0 to 700 V at 60 Hz Accuracy: $\pm 3\%$ of FS
	Ac amps	Range: 0 to 1000 A at 60 Hz Accuracy: $\pm 3\%$ of FS
Weston, Model 749 (horizontal position)	Ac volts	Range: 0 to 600 V Accuracy: $\pm 3\%$ of FS at 60 Hz $\pm 5\%$ of FS at 400 Hz
	Ac amps	Range: 0 to 300 A Accuracy: $\pm 3\%$ of FS at 60 Hz $\pm 5\%$ of FS at 400 Hz
Weston, Model 901 (horizontal position)	Dc volts	Range: 0 to 1000 V Accuracy: $\pm 0.5\%$ of FS
	Dc amps	Range: 100 μ A to 50 A Accuracy: $\pm 0.5\%$ of FS

Table 1. Calibration Description - Continued

Manufacturer and model	Test instrument	
	Parameters	Performance specifications
Weston, Model 904 (horizontal position)	Ac volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS, 50 to 125 Hz $\pm 1\%$ of FS, 125 to 450 Hz
	Ac amps	Range: 0 to 200 A, 25 to 500 Hz Accuracy: $\pm 0.5\%$ of FS
Weston, Model 931 (horizontal position)	Dc volts	Range: 0 to 750 V Accuracy: $\pm 0.5\%$ of FS
	Dc amps	Range: 0 to 50 A Accuracy: $\pm 0.5\%$ of FS

SECTION II EQUIPMENT REQUIREMENTS

4. Equipment Required. Table 2 identifies the specific equipment to be used in this calibration procedure. This equipment is issued with Secondary Transfer Calibration Standards Set AN/GSM-286, AN/GSM-287 and AN/GSM-705. Alternate items may be used by the calibrating activity when the equipment listed in table 2 is not available. The items selected must be verified to perform satisfactorily prior to use and must bear evidence of current calibration. The equipment must meet or exceed the minimum use specifications listed in table 2. The accuracies listed in table 2 provide a four-to-one ratio between the standard and TI. Where the four-to-one ratio cannot be met, the actual accuracy of the equipment selected is shown in parenthesis.

5. Accessories Required. The accessories listed in table 3 are issued as indicated in paragraph 4 above and are used in this calibration procedure. When necessary these items may be substituted by equivalent items, unless specifically prohibited.

Table 2. Minimum Specifications of Equipment Required

Common name	Minimum use specifications	Manufacturer and model (part number)
CALIBRATOR	Range: 0 to 773 V 15 to 2500 Hz Accuracy: $\pm 0.125\%$	Fluke, Model 5720A (5720A) (p/o MIS-35947); w amplifier, Fluke 5725A/AR (5725A/AR)
DC CURRENT SHUNT	Range: 0 to 51 A Accuracy: $\pm 0.01\%$	Guildline, Model 9711 (7912323)
MULTIMETER	Range: Dc: 0 to 101 mV Ac: 0 to 1.05 V Accuracy: $\pm .005\%$	Agilent, Model 3458A (3458A)
VOLTAGE STANDARD	Range: High 0 to 200 Vac Low 0 to 30 Vac	Holt Instrument, Model 97717 (97717)

Table 3. Accessories Required

Common name	Description (part number)
DC POWER SUPPLY NO. 1	Elgar, Model DCS40-30EM10 (13589313)
DC POWER SUPPLY NO. 2	Sorenson, Model 20-250A (MIS-35935)
DECADE RESISTOR	Winslow, Model 336 (7907234) or Clarostat, Model 240C (240C)

SECTION III CALIBRATION PROCESS

6. Preliminary Instructions

a. The instructions outlined in paragraphs 6 and 7 are preparatory to the calibration process. Personnel should become familiar with the entire bulletin before beginning the calibration.

b. Items of equipment used in this procedure are referenced within the text by common name as listed in tables 2 and 3.

c. Unless otherwise specified, verify the result of each test and, whenever the test requirement is not met, take corrective action before continuing with the calibration. Adjustments required to calibrate each TI are included in this procedure. Additional maintenance information is contained in the manufacturer's manual for each TI.

d. This is a general procedure which provides instructions for the calibration of any instrument within the series. Each instrument requires a check for meter tracking and linearity on one range and full-scale accuracy on the remaining ranges.

e. Unless otherwise specified, all controls and control settings refer to the TI.

7. Equipment Setup

WARNING

HIGH VOLTAGE is used or exposed during the performance of this calibration. DEATH ON CONTACT may result if personnel fail to observe safety precautions. REDUCE OUTPUT(S) to minimum after each step within the performance check where applicable.

a. Place TI in horizontal position for calibration.

b. Adjust meter mechanical zero adjustment for zero meter indication if required.

8. DC Volts

a. Performance Check

- (1) Set TI function switch (if applicable) to dc volts (millivolts) and set range switch to lowest range.
- (2) Connect calibrator to TI observing polarity.
- (3) Adjust calibrator for full-scale indication on TI. Calibrator will indicate within limits specified under accuracy in table 4 for TI being calibrated.
- (4) Repeat technique of (1) and (3) above for remaining ranges.

NOTE

Perform tracking and linearity check on a convenient range at cardinal points approximately two-thirds and one-third of full scale. Indications will be within stated \pm percent of full scale for each cardinal point.

b. Adjustments. No adjustments can be made.

Table 4. Dc Voltage

Test instrument range	Calibrator indications (V)			
	TS-433/U		TS-340/U and Weston, Models 430, 455, 622 series, 901 and 931	
	$\pm 0.25\%$		$\pm 0.5\%$	
	Min	Max	Min	Max
1 mV	---	---	0.995	1.005
2 mV	---	---	1.99	2.01
5 mV	---	---	4.975	5.025
10 mV	---	---	9.95	10.05
20 mV	---	---	1.99	2.01
50 mV	---	---	4.975	5.025
100 mV	---	---	9.95	10.05
200 mV	---	---	0.1990	0.201
500 mV	---	---	0.4975	0.5025
1000 mV	---	---	0.9950	1.0050
2000 mV	---	---	1.9900	2.0100
1.5 V	---	---	1.4925	1.5075
2 V	---	---	1.99	2.01
2.8 V	---	---	2.786	2.814
3 V	2.9925	3.0075	2.985	3.015
5 V	---	---	4.975	5.025
7.5 V	---	---	7.462	7.538
10 V	---	---	9.95	10.05
15 V	14.9625	15.0375	14.925	15.075
20 V	---	---	19.9	20.1
30 V	---	---	29.85	30.15
50 V	---	---	49.75	50.25
60 V	---	---	59.70	60.30

Table 4. Dc Voltage - Continued

Test instrument range	Calibrator indications (V)			
	TS-433/U		TS-340/U and Weston, Models 430, 455, 622 series, 901 and 931	
	±0.25%		±0.5%	
	Min	Max	Min	Max
75 V	---	---	74.625	75.375
100 V	---	---	99.50	100.5
125 V	---	---	124.37	125.63
150 V	149.625	150.375	149.25	150.75
200 V	---	---	199.0	210.0
250 V	---	---	248.75	251.23
300 V	---	---	298.5	301.5
400 V	---	---	398.0	402.0
450 V	---	---	447.75	452.25
500 V	---	---	497.5	502.5
600 V	---	---	597.0	603.0
750 V	---	---	746.25	753.75
1000 V	---	---	995.0	1005.0

9. Dc Amps

a. Performance Check

- (1) Set TI function switch (if applicable) to dc amps and set range switch to lowest range.
- (2) Connect equipment as shown in figure 1.

NOTE

Position dc current shunt range plugs as required for range being calibrated. Also set decade resistor controls as required for current limiting and remove when current exceeds decade resistor current capability.

- (3) Adjust dc power supply no. 1 and decade resistor as required for full-scale indication on TI meter. Multimeter will indicate within limits specified under accuracy in table 5 for TI being calibrated.

NOTE

Perform tracking and linearity check on a convenient range at cardinal points two-thirds and one-third of full scale. Indications will be within stated \pm percent of full scale for each cardinal point.

- (4) Repeat technique of (1) and (3) above for remaining ranges.

b. Adjustments. No adjustments can be made.

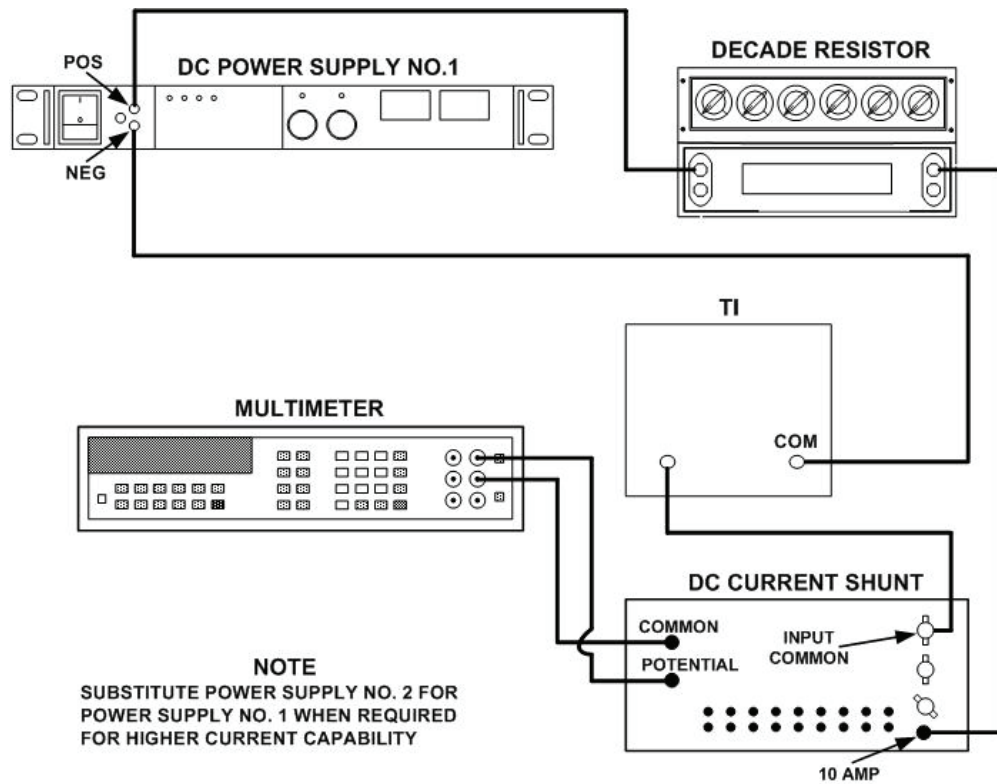


Figure 1. Dc current - equipment setup.

Table 5. Dc Current

Test instrument range	Multimeter indications (mV dc)			
	SRI, Models C-CILKI and C-CILORD		ME-221/U and Weston, Models 430, 901, 931, and 622 series	
	±0.25%		±0.5%	
	Min	Max	Min	Max
5 μ A	---	---	49.75	50.25
10 μ A	---	---	99.5	100.5
15 μ A	---	---	14.925	15.075
20 μ A	---	---	19.90	20.10
30 μ A	---	---	29.85	30.15
50 μ A	---	---	49.75	50.25
100 μ A	---	---	99.5	100.5
150 μ A	---	---	14.925	15.075
200 μ A	---	---	19.90	20.10
500 μ A	---	---	49.75	50.25
1000 μ A	---	---	99.5	100.5
0.03 mA	---	---	29.85	30.15
0.05 mA	49.875	50.125	---	---
0.1 mA	99.75	100.25	99.5	100.5
0.2 mA	---	---	19.90	20.10
0.3 mA	---	---	29.85	30.15
0.5 mA	49.875	50.125	49.75	50.25

Table 5. Dc Current - Continued

Test instrument range	Multimeter indications (mV dc)			
	SRI, Models C-CILKI and C-CILORD		ME-221/U and Weston, Models 430, 901, 931, and 622 series	
	±0.25%		±0.5%	
	Min	Max	Min	Max
1 mA	99.75	100.25	99.5	100.5
1.5 mA	---	---	14.925	15.075
2 mA	19.95	20.05	19.90	20.10
3 mA	---	---	29.85	30.15
5 mA	49.875	50.125	49.75	50.25
7.5 mA	---	---	74.625	75.375
10 mA	99.75	100.25	99.5	100.5
15 mA	14.963	15.037	14.925	15.075
20 mA	19.95	20.05	19.90	20.10
30 mA	29.925	30.075	29.85	30.15
50 mA	49.875	50.125	49.75	50.25
75 mA	74.813	75.187	---	---
100 mA	99.75	100.25	99.5	100.5
150 mA	14.963	15.037	14.925	15.075
200 mA	19.95	20.05	19.90	20.10
300 mA	---	---	29.85	30.15
500 mA	49.875	50.125	49.75	50.25
750 mA	74.813	75.187	74.625	75.375
0.05 A	---	---	49.75	50.25
0.1 A	---	---	99.5	100.5
0.15 A	---	---	14.925	15.075
0.5 A	---	---	49.75	50.25
1 A	99.75	100.25	99.5	100.5
1.5 A	14.963	15.037	14.925	15.075
2 A	19.95	20.05	19.90	20.10
2.5 A	---	---	24.875	25.125
3 A	29.925	30.075	29.85	30.15
5 A	49.875	50.125	49.75	50.25
7.5 A	74.813	75.187	74.625	75.375
10 A	---	---	99.5	100.5
15 A	---	---	14.925	15.075
20 A	19.95	20.05	19.90	20.10
25 A	---	---	24.875	25.125
30 A	29.925	30.075	29.85	30.15
50 A	---	---	49.75	50.25

10. Ac Volts

a. Performance Check

(1) Set TI function switch (if applicable) to ac volts and set range switch to lowest range.

(2) Connect calibrator to TI.

(3) Adjust calibrator to mid-frequency of frequency range (if applicable) as listed in table 6 and voltage output for full-scale indication on TI. Calibrator will indicate within limits specified under accuracy in table 6 for TI being calibrated.

(4) Repeat (3) above at low and high frequency listed for TI.

(5) Repeat technique of (1), (3), and (4) above for remaining ranges.

NOTE

Perform tracking and linearity check on a convenient range at cardinal points approximately two-thirds and one-third of full scale. Indications will be within stated \pm percent of full scale for each cardinal point.

b. Adjustments. No adjustments can be made.

Table 6. Ac Voltage

Test instrument range	Calibrator indications (V ac)							
	Weston, Model 904 50 to 125 Hz TS-340 25 to 400 Hz Weston, Model 430 25 to 2000 Hz Weston, Model 455 25 to 1000 Hz		Weston, Model 433 25 to 125 Hz Westinghouse, Model PY-4 15 to 200 Hz		Weston, Model 904 125 to 450 Hz		Weston, Model 433 125 to 2500 Hz	
	$\pm 0.5\%$		$\pm 0.75\%$		$\pm 1\%$		$\pm 1.25\%$	
	Min	Max	Min	Max	Min	Max	Min	Max
3	2.985	3.015	---	---	2.97	3.03	---	---
4	---	---	---	---	---	---	---	---
5	---	---	4.9625	5.0375	---	---	4.937	5.063
7.5	7.4625	7.5375	---	---	7.425	7.575	---	---
8	---	---	---	---	---	---	---	---
10	---	---	9.925	10.075	---	---	9.875	10.125
15	14.925	15.075	14.888	15.112	14.85	15.15	14.812	15.188
20	---	---	19.85	20.15	---	---	19.75	20.25
30	29.85	30.15	29.775	30.225	29.7	30.3	29.625	30.375
50	49.75	50.25	49.625	50.375	---	---	49.375	50.625
60	---	---	59.550	60.450	---	---	59.45	60.75
75	74.625	75.375	74.438	75.562	74.25	75.75	74.062	75.937
125	---	---	124.06	125.94	---	---	123.44	126.56
150	149.25	150.75	148.88	151.12	148.5	151.5	148.12	151.88
175	---	---	---	---	---	---	---	---
250	---	---	248.12	251.88	---	---	246.88	253.12
300	298.5	301.5	297.75	301.25	297.0	303.0	296.25	303.75
350	---	---	---	---	---	---	---	---
400	389.0	402.0	---	---	---	---	---	---
450	---	---	446.62	453.38	---	---	444.38	455.62
600	---	---	595.50	604.50	---	---	592.50	607.50
700	---	---	---	---	---	---	---	---
750	746.25	753.75	744.38	755.62	742.5	757.5	740.62	759.38

Table 6. Ac Voltage- Continued

Test instrument range	Calibrator indications (V ac)					
	Weston, Model 528 25 to 125 Hz		General Electric, Model AK-4, Weston, Models 749 and 633-VA1 At 60 Hz only ME-489/U		Weston, Model 749 400 Hz only ME-79/USM-33 ME-79A/USM-33 50 to 1000 Hz	
	±2%		±3%		±5%	
	Min	Max	Min	Max	Min	Max
3	2.94	3.06	---	---	---	---
4	3.92	4.08	---	---	---	---
5	---	---	---	---	---	---
7.5	---	---	---	---	---	---
8	7.84	8.16	---	---	---	---
10	---	---	---	---	---	---
15	14.7	15.3	---	---	---	---
20	---	---	---	---	---	---
30	---	---	---	---	---	---
50	---	---	---	---	---	---
60	---	---	---	---	---	---
75	---	---	---	---	---	---
125	---	---	---	---	---	---
150	147	153	145.5	154.5	142.5	157.5
175	---	---	169.75	180.25	---	---
250	---	---	---	---	---	---
300	294.0	306.0	291.0	309.0	285.0	315.0
350	---	---	339.5	360.5	---	---
400	---	---	---	---	---	---
450	---	---	---	---	---	---
600	588.0	612.0	582.0	618.0	570.0	630.0
700	---	---	679.0	721.0	---	---
750	---	---	727.5	772.5	---	---

11. Ac Amps

a. Performance Check

(1) Set TI function switch (if applicable) to ac current and set range switch to lowest range.

(2) Connect equipment as shown in figure 2.

(3) Adjust calibrator frequency for 60 Hz and voltage output as required to obtain full-scale indication on TI. Multimeter will indicate within limits specified under accuracy in table 7 for TI being calibrated.

(4) Repeat (3) above at low (50 Hz) and high (as applicable) (1000 Hz maximum) frequency listed for TI.

(5) Repeat technique of (1), (3), and (4) above for remaining ranges.

NOTE

Perform tracking and linearity check on a convenient range at cardinal points approximately two-thirds and one-third of full scale. Indications will be within stated \pm percent of full scale for each cardinal point.

b. **Adjustments.** No adjustments can be made.

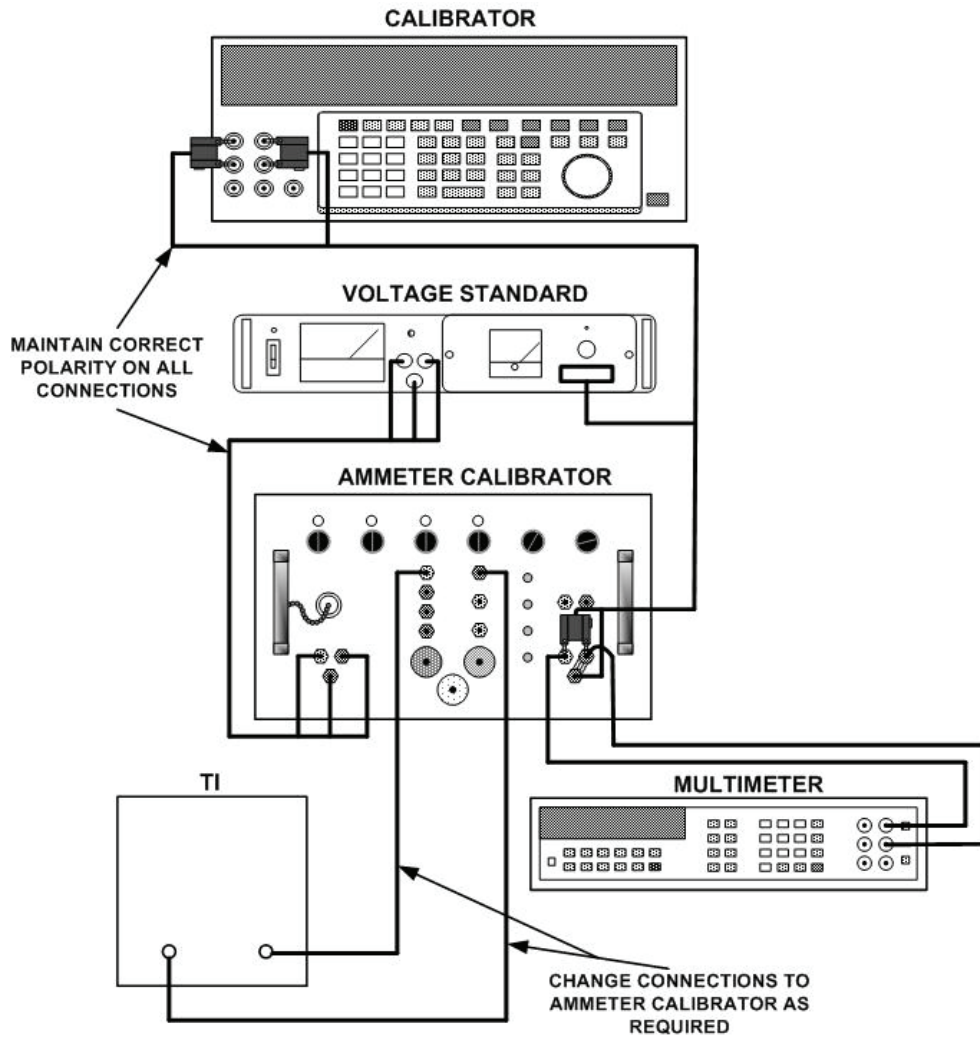


Figure 2. Ac current - equipment setup.

Table 7. Ac Current

Test instrument range	Multimeter indications (V ac)							
	Westinghouse, Model PA5 20 to 135 Hz ME-65/U and ME-65A/U, Weston Models 155 and 904 25 to 500 Hz		Weston, Model 528 25 to 500 Hz		General Electric, Model AK-4 Weston, Models 633 Series and 749 At 60 Hz only ME-489/U		Weston, Model 749 at 400 Hz Only ME-79/USM-33 ME-79A/USM-33 50 to 1000 Hz	
	±0.5%		±2%		±3%		±5%	
	Min	Max	Min	Max	Min	Max	Min	Max
15 mA	---	---	0.98	1.02	---	---	---	---
50 mA	---	---	0.98	1.02	---	---	---	---
100 mA	---	---	0.98	1.02	---	---	---	---
.5 A	0.995	1.005	0.98	1.02	---	---	---	---
1 A	0.995	1.005	0.98	1.02	---	---	---	---
2 A	0.995	1.005	---	---	---	---	---	---
2.5 A	0.995	1.005	---	---	---	---	---	---
3 A	0.995	1.005	0.98	1.02	---	---	---	---
5 A	0.995	1.005	0.98	1.02	---	---	---	---
6 A	---	---	---	---	0.97	1.03	0.95	1.05
10 A	0.995	1.005	0.98	1.02	0.97	1.03	---	---
15 A	0.995	1.005	0.98	1.02	0.97	1.03	0.95	1.05
20 A	0.995	1.005	---	---	---	---	---	---
25 A	0.995	1.005	---	---	0.97	1.03	---	---
30 A	---	---	0.98	1.02	0.97	1.03	0.95	1.05
50 A	0.995	1.005	0.98	1.02	0.97	1.03	---	---
60 A	---	---	---	---	0.97	1.03	0.95	1.05
100 A ¹	0.995	1.005	---	---	0.97	1.03	---	---
150 A ¹	---	---	---	---	0.97	1.03	0.95	1.05
200 A ¹	0.995	1.005	---	---	---	---	---	---
250 A ¹	---	---	---	---	0.97	1.03	---	---
300 A ¹	---	---	---	---	0.97	1.03	0.95	1.05
500 A ¹	---	---	---	---	0.97	1.03	---	---
800 A ¹	---	---	---	---	0.97	1.03	---	---
1000 A ¹	---	---	---	---	0.97	1.03	---	---
2000 A ¹	---	---	---	---	0.97	1.03	---	---

¹Check these ranges at the maximum capability of the ac power supply and ac current calibrator.

12. Final Procedure

- a. Deenergize and disconnect all equipment and reinstall protective cover on TI.
- b. Annotate and affix DA Label/Form in accordance with TB 750-25.

By Order of the Secretary of the Army:

Official:



JOYCE E. MORROW
*Administrative Assistant to the
Secretary of the Army*

0730503

GEORGE W. CASEY, JR.
*General, United States Army
Chief of Staff*

Distribution:

To be distributed in accordance with the initial distribution number (IDN) 343451, requirements for calibration procedure TB 9-6625-2146-24.

INSTRUCTIONS FOR SUBMITTING AN ELECTRONIC 2028

The following format must be used if submitting an electronic 2028. The subject line must be exactly the same and all fields must be included; however, only the following fields are mandatory: 1, 3, 4, 5, 6, 7, 8, 9, 10, 13, 15, 16, 17, and 27.

From: "Whomever" whomever@redstone.army.mil
To: <2028@redstone.army.mil

Subject: DA Form 2028

1. **From:** Joe Smith
2. **Unit:** home
3. **Address:** 4300 Park
4. **City:** Hometown
5. **St:** MO
6. **Zip:** 77777
7. **Date Sent:** 19-OCT -93
8. **Pub no:** 55-2840-229-23
9. **Pub Title:** TM
10. **Publication Date:** 04-JUL-85
11. **Change Number:** 7
12. **Submitter Rank:** MSG
13. **Submitter FName:** Joe
14. **Submitter MName:** T
15. **Submitter LName:** Smith
16. **Submitter Phone:** 123-123-1234
17. **Problem:** 1
18. **Page:** 2
19. **Paragraph:** 3
20. **Line:** 4
21. **NSN:** 5
22. **Reference:** 6
23. **Figure:** 7
24. **Table:** 8
25. **Item:** 9
26. **Total:** 123
27. **Text**

This is the text for the problem below line 27.

